

**Quantitative Analysis for Ethanol & Qualitative Analysis for Other Volatiles**

*Analytical Method(s): 1.0*

*Device: Hamilton MICROLAB 600 Liquid Processor/Dilutor Serial Number: ML600HC11378*

**Volatiles Quality Assurance Controls**

**Run Date: 09/05/18-09/06/18**

Calibration Date: 09/05/18

Control level	Expiration	Lot #	Target Value	Acceptable Range	Overall Results
Level 1	Jan-22	1801036	0.0812	0.0731-0.0893	0.0793 g/100cc
					0.0827 g/100cc
					0.2011 g/100cc
Level 2	Mar-22	1803028	0.2035	0.1832-0.2238	0.2011 g/100cc g/100cc g/100cc
<b>Multi-Component mixture:</b>		<b>Exp date: Sept 2020</b>	<b>Lot #</b>	<b>FN06041502</b>	<b>OK</b>
<b>Curve Fit:</b>		<b>Column 1</b>	<b>0.99999</b>	<b>Column2</b>	<b>0.99999</b>

Ethanol Calibration Reference Material								
Calibrator level	Expiration	Ceriliant Lot #	Target Value	Acceptable Range	Column 1	Column 2	Precision	Mean
0.050	Jul-19	FN06231406	0.050	0.045 - 0.055	0.0504	0.0509	0.0005	0.0506
0.080			0.080	0.072 - 0.088			0	#DIV/0!
0.100	Aug-21	FN08101601	0.100	0.090 - 0.110	0.0994	0.0997	0.0003	0.0995
0.200	Dec-19	FN12011401	0.200	0.180 - 0.220	0.1996	0.1989	0.0007	0.1992
0.300	Feb-21	FN02121601	0.300	0.270 - 0.330	0.3008	0.3002	0.0006	0.3005
0.400			0.400	0.360 - 0.440			0	#DIV/0!
0.500	Sep-21	FN07031402	0.500	0.450 - 0.550	0.4997	0.5003	0.0006	0.5

Aqueous Controls					
Control level	Expiration	Ceriliant Lot #	Target Value	Acceptable Range	Overall Results
0.080	May-22	FN04171701	0.08000	0.076 - 0.084	0.080 g/100cc

Issued: 4/22/2015


~Any information on this document can be changed for laboratory use, except for the precision and mean determination formulas.

Volatiles QA/QC data spreadsheet Rev 5  
Issuing Authority: Quality Manager

*jk*

**Worklist: 2676**

<u>LAB CASE</u>	<u>ITEM</u>	<u>TASK ID</u>	<u>DESCRIPTION</u>
M2018-4314	1	125207	Alcohol Analysis
M2018-4316	1	125318	Alcohol Analysis
M2018-4317	1	125321	Alcohol Analysis
M2018-4324	3	125390	Alcohol Analysis
M2018-4324	4	125394	Alcohol Analysis
M2018-4330	1	125395	Alcohol Analysis
M2018-4330	2	125399	Alcohol Analysis
M2018-4331	1	125403	Alcohol Analysis
M2018-4332	1	125407	Alcohol Analysis
M2018-4346	1	125496	Alcohol Analysis
M2018-4347	1	125497	Alcohol Analysis
M2018-4348	1	125498	Alcohol Analysis
M2018-4370	1	125580	Alcohol Analysis
M2018-4375	1	125600	Alcohol Analysis
M2018-4376	1	125601	Alcohol Analysis
M2018-4378	1	125604	Alcohol Analysis
M2018-4379	1	125608	Alcohol Analysis
M2018-4387	1	125622	Alcohol Analysis
M2018-4411	1	125685	Alcohol Analysis

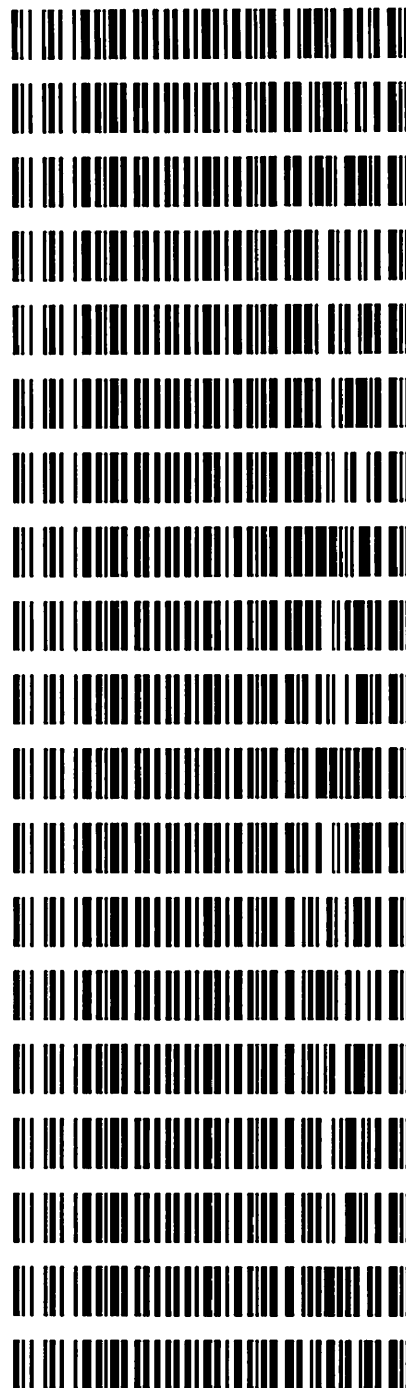

=====  
Calibration Table  
=====

-----  
General Calibration Setting  
-----

Calib. Data Modified : Wednesday, September 05, 2018 3:47:55 PM  
Signals calculated separately : No

Rel. Reference Window : 0.000 %  
Abs. Reference Window : 0.100 min  
Rel. Non-ref. Window : 0.000 %  
Abs. Non-ref. Window : 0.100 min  
Uncalibrated Peaks : not reported  
Partial Calibration : Yes, identified peaks are recalibrated  
Correct All Ret. Times: No, only for identified peaks

Curve Type : Linear  
Origin : Ignored  
Weight : Equal

Recalibration Settings:  
Average Response : Average all calibrations  
Average Retention Time: Floating Average New 75%

Calibration Report Options :  
Printout of recalibrations within a sequence:  
    Calibration Table after Recalibration  
    Normal Report after Recalibration  
If the sequence is done with bracketing:  
    Results of first cycle (ending previous bracket)

Default Sample ISTD Information (if not set in sample table):

ISTD #	ISTD Amount [g/100cc]	Name
1	1.00000	n-propanol
2	1.00000	n-propanol

-----  
Signal Details  
-----

Signal 1: FID1 A, Front Signal  
Signal 2: FID2 B, Back Signal  
-----

-----  
Overview Table  
-----

JL

RT	Sig	Lvl	Amount [g/100cc]	Area	Rsp.Factor	Ref	ISTD #	Compound
2.586	1	1	1.00000	3.69669	2.70512e-1	No	No 1	methanol
2.809	1	1	1.00000	4.26100	2.34687e-1	No	No 2	Acetaldehyde
2.977	2	1	1.00000	4.26100	2.34687e-1	No	No 2	Acetaldehyde
3.075	1	1	5.00000e-2	4.59817	1.08739e-2	No	No 1	ethanol
			1.00000e-1	9.32346	1.07256e-2			
			2.00000e-1	18.41389	1.08614e-2			
			3.00000e-1	27.45264	1.09279e-2			
			5.00000e-1	46.08223	1.08502e-2			
3.388	2	1	1.00000	4.26062	2.34707e-1	No	No 2	methanol
3.628	1	1	1.00000	9.73055	1.02769e-1	No	No 1	isopropyl alcohol
4.285	2	1	5.00000e-2	4.66852	1.07100e-2	No	No 2	ethanol
			1.00000e-1	9.64956	1.03632e-2			
			2.00000e-1	19.22962	1.04006e-2			
			3.00000e-1	28.79560	1.04183e-2			
			5.00000e-1	48.70642	1.02656e-2			
4.308	1	1	1.00000	6.49940	1.53860e-1	No	No 1	acetone
4.620	1	1	1.00000	48.17749	2.07566e-2	No	Yes 1	n-propanol
			1.00000	49.21605	2.03186e-2			
			1.00000	48.27000	2.07168e-2			
			1.00000	47.70254	2.09632e-2			
			1.00000	48.15673	2.07655e-2			
4.661	2	1	1.00000	6.89301	1.45075e-1	No	No 2	acetone
4.969	2	1	1.00000	10.70642	9.34019e-2	No	No 2	isopropyl alcohol
7.550	2	1	1.00000	50.14548	1.99420e-2	No	Yes 2	n-propanol
			1.00000	50.94972	1.96272e-2			
			1.00000	49.87467	2.00503e-2			
			1.00000	49.17295	2.03364e-2			
			1.00000	49.65463	2.01391e-2			


Peak Sum Table

\*\*\*No Entries in table\*\*\*

1 Warnings or Errors :


Warning : Curve requires more calibration points., (methanol)

Calibration Curves

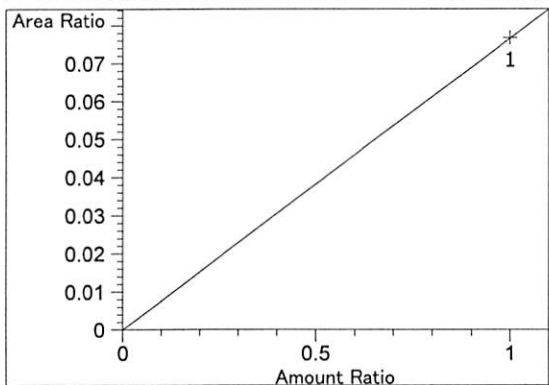


methanol at exp. RT: 2.586  
 FID1 A, Front Signal  
 Correlation: 1.00000  
 Residual Std. Dev.: 0.00000  
 Formula:  $y = mx + b$   
 m: 7.67307e-2  
 b: 0.00000  
 x: Amount Ratio  
 y: Area Ratio


JK

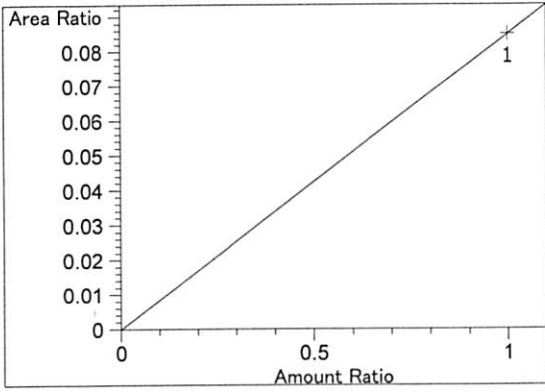


Acetaldehyde at exp. RT: 2.809  
FID1 A, Front Signal  
Correlation: 1.00000  
Residual Std. Dev.: 0.00000  
Formula:  $y = mx + b$   
m:  $8.49728e-2$   
b: 0.00000  
x: Amount Ratio  
y: Area Ratio

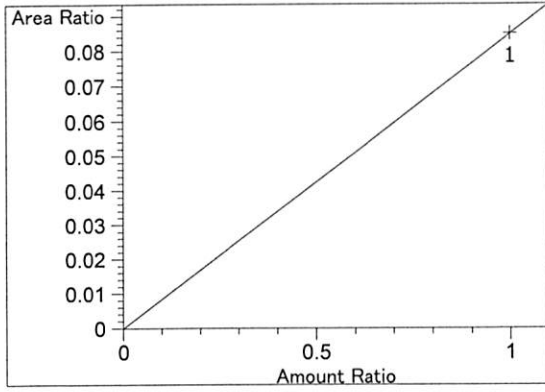

Acetaldehyde at exp. RT: 2.977  
FID2 B, Back Signal  
Correlation: 1.00000  
Residual Std. Dev.: 0.00000  
Formula:  $y = mx + b$   
m:  $8.49728e-2$   
b: 0.00000  
x: Amount Ratio  
y: Area Ratio

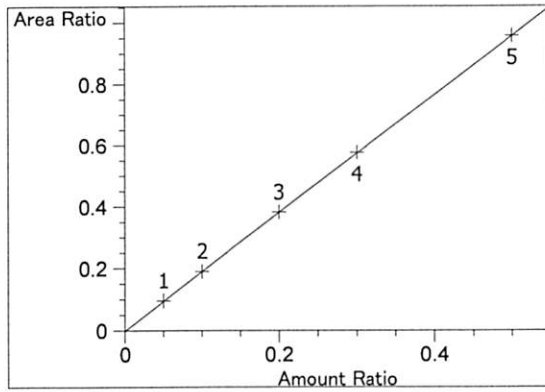


ethanol at exp. RT: 3.075  
FID1 A, Front Signal  
Correlation: 0.99999  
Residual Std. Dev.: 0.00128  
Formula:  $y = mx + b$   
m: 1.91721  
b:  $-1.20246e-3$   
x: Amount Ratio  
y: Area Ratio

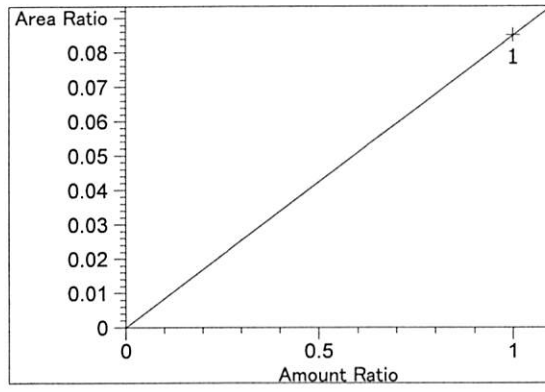


methanol at exp. RT: 3.388  
FID2 B, Back Signal  
Correlation: 1.00000  
Residual Std. Dev.: 0.00000  
Formula:  $y = mx + b$   
m:  $8.49653e-2$   
b: 0.00000  
x: Amount Ratio  
y: Area Ratio


*JK*

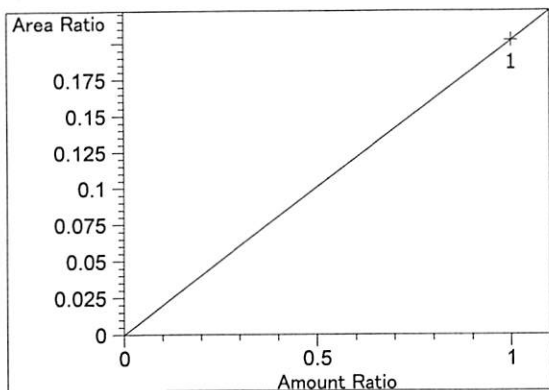


isopropyl alcohol at exp. RT: 3.628  
 FID1 A, Front Signal  
 Correlation: 1.00000  
 Residual Std. Dev.: 0.00000  
 Formula:  $y = mx + b$   
 m: 2.01973e-1  
 b: 0.00000  
 x: Amount Ratio  
 y: Area Ratio

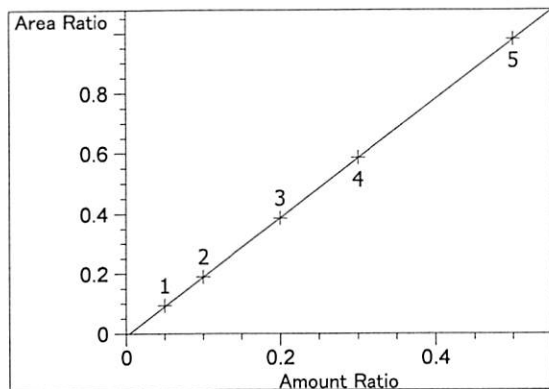

ethanol at exp. RT: 4.285  
 FID2 B, Back Signal  
 Correlation: 0.99999  
 Residual Std. Dev.: 0.00169  
 Formula:  $y = mx + b$   
 m: 1.97570  
 b: -7.50104e-3  
 x: Amount Ratio  
 y: Area Ratio

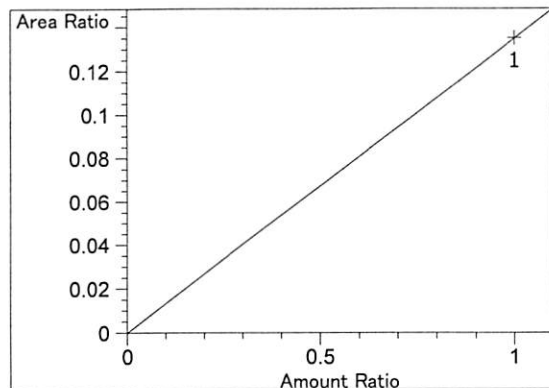


acetone at exp. RT: 4.308  
 FID1 A, Front Signal  
 Correlation: 1.00000  
 Residual Std. Dev.: 0.00000  
 Formula:  $y = mx + b$   
 m: 1.34905e-1  
 b: 0.00000  
 x: Amount Ratio  
 y: Area Ratio

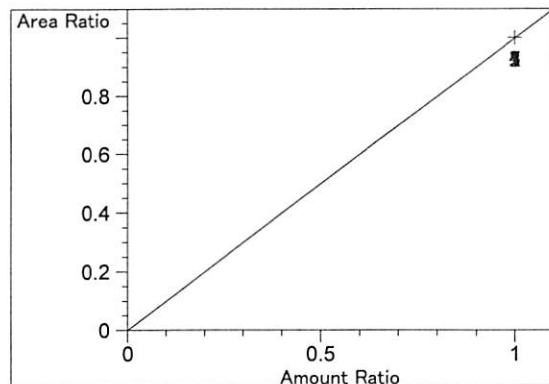


n-propanol at exp. RT: 4.620  
 FID1 A, Front Signal  
 Correlation: 1.00000  
 Residual Std. Dev.: 0.00000  
 Formula:  $y = mx + b$   
 m: 1.00000  
 b: 0.00000  
 x: Amount Ratio  
 y: Area Ratio


JK

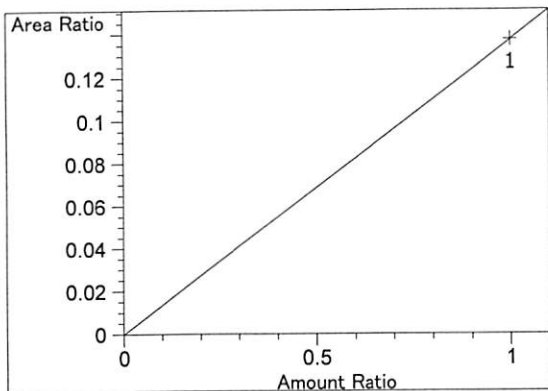

acetone at exp. RT: 4.661  
FID2 B, Back Signal  
Correlation: 1.00000  
Residual Std. Dev.: 0.00000  
Formula:  $y = mx + b$   
m: 1.37460e-1  
b: 0.00000  
x: Amount Ratio  
y: Area Ratio

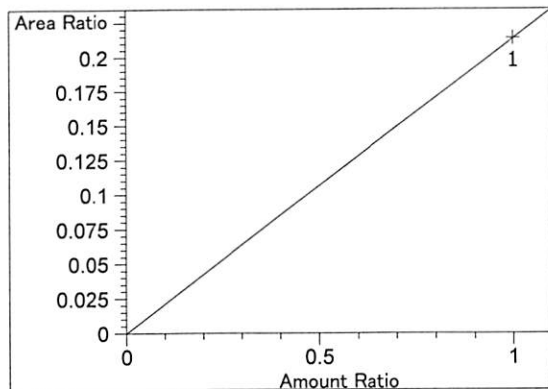

isopropyl alcohol at exp. RT: 4.969  
FID2 B, Back Signal  
Correlation: 1.00000  
Residual Std. Dev.: 0.00000  
Formula:  $y = mx + b$   
m: 2.13507e-1  
b: 0.00000  
x: Amount Ratio  
y: Area Ratio

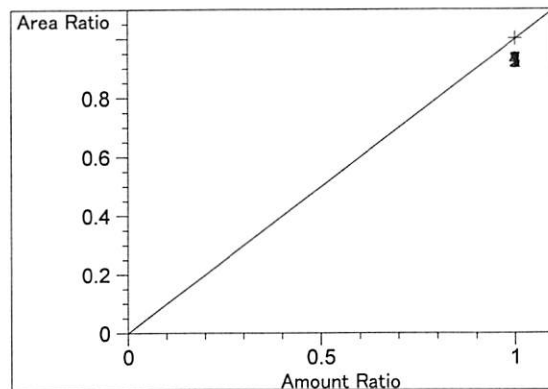


n-propanol at exp. RT: 7.550  
FID2 B, Back Signal  
Correlation: 1.00000  
Residual Std. Dev.: 0.00000  
Formula:  $y = mx + b$   
m: 1.00000  
b: 0.00000  
x: Amount Ratio  
y: Area Ratio

=====

JK

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.050 FN06231406  
 Laboratory : Meridian  
 Injection Date : Sep 5, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

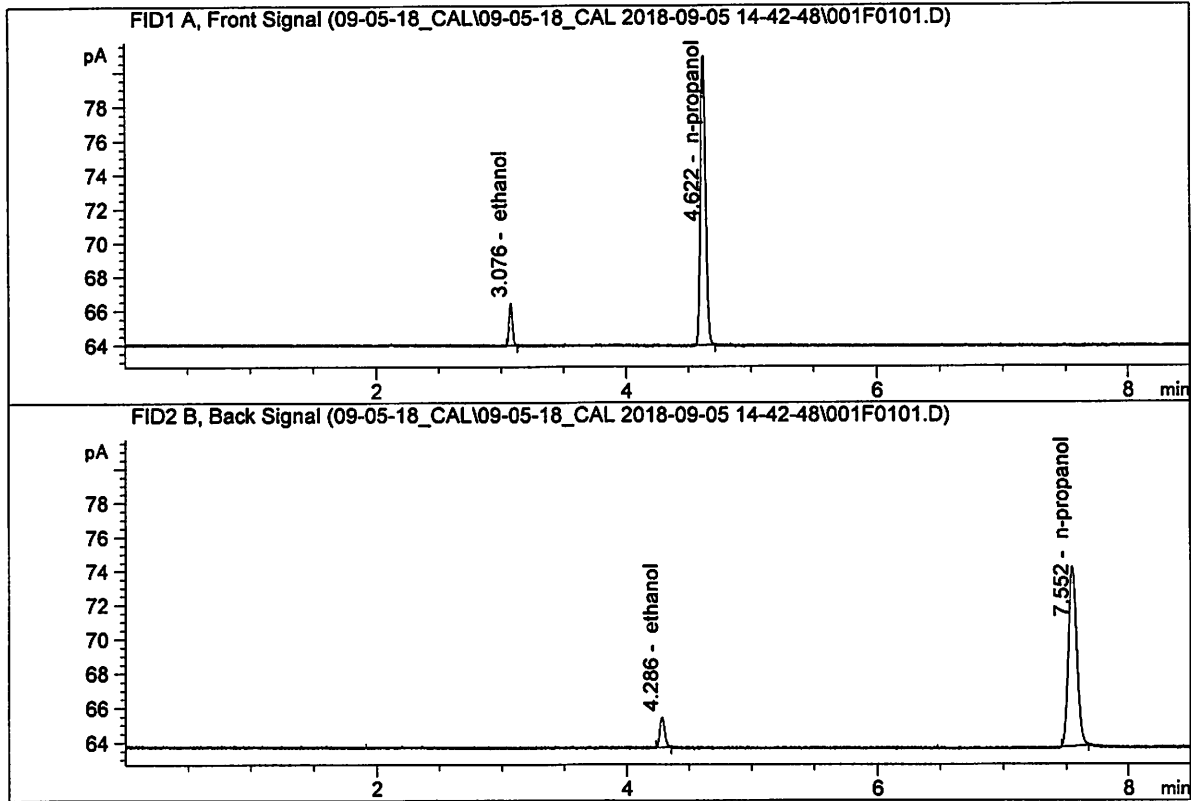


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	4.59817	0.0504	g/100cc
2.	Ethanol	Column 2:	4.66852	0.0509	g/100cc
3.	n-Propanol	Column 1:	48.17749	1.0000	g/100cc
4.	n-Propanol	Column 2:	50.14548	1.0000	g/100cc



ISP Forensic Services Blood Alcohol Report


Sample Name : 0.100 FN08101601  
 Laboratory : Meridian  
 Injection Date : Sep 5, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

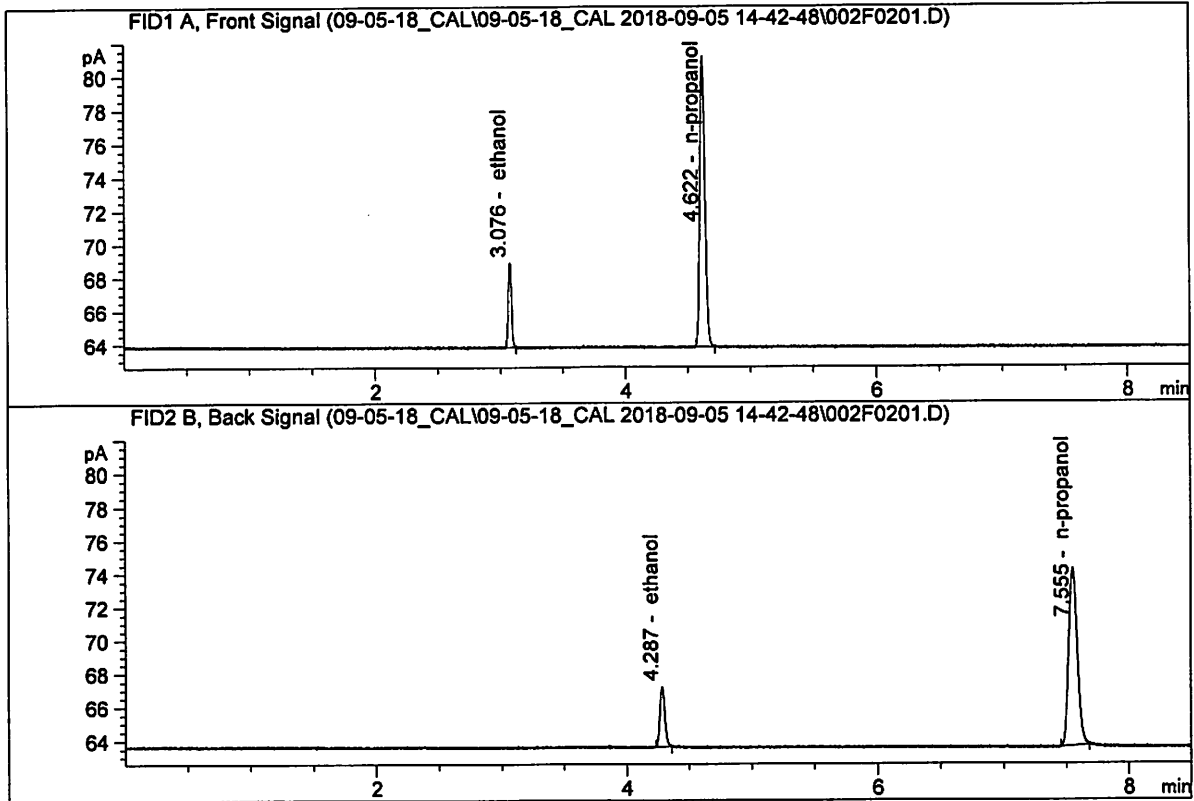

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	9.32346	0.0994	g/100cc
2.	Ethanol	Column 2:	9.64956	0.0997	g/100cc
3.	n-Propanol	Column 1:	49.21605	1.0000	g/100cc
4.	n-Propanol	Column 2:	50.94972	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.200 FN12011401  
 Laboratory : Meridian  
 Injection Date : Sep 5, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

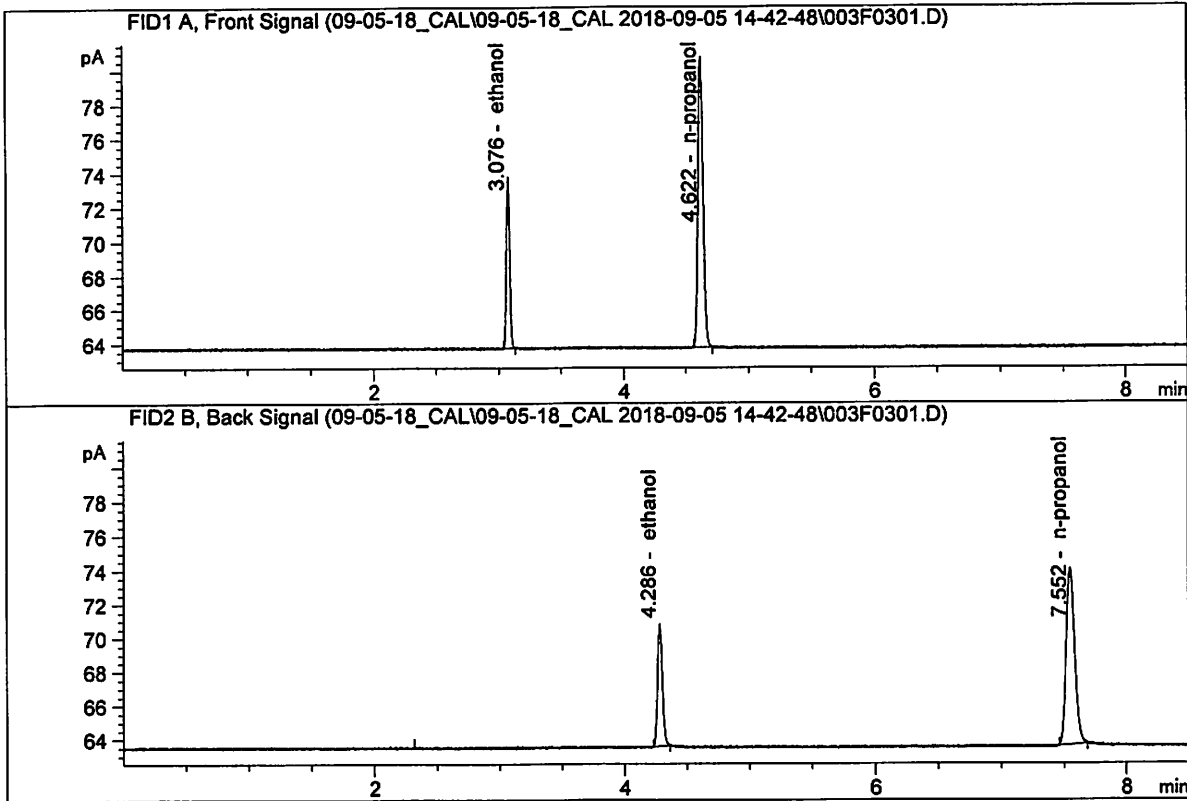


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	18.41389	0.1996	g/100cc
2.	Ethanol	Column 2:	19.22962	0.1989	g/100cc
3.	n-Propanol	Column 1:	48.27000	1.0000	g/100cc
4.	n-Propanol	Column 2:	49.87467	1.0000	g/100cc

JK

ISP Forensic Services Blood Alcohol Report


Sample Name : 0.300 FN02121601  
 Laboratory : Meridian  
 Injection Date : Sep 5, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

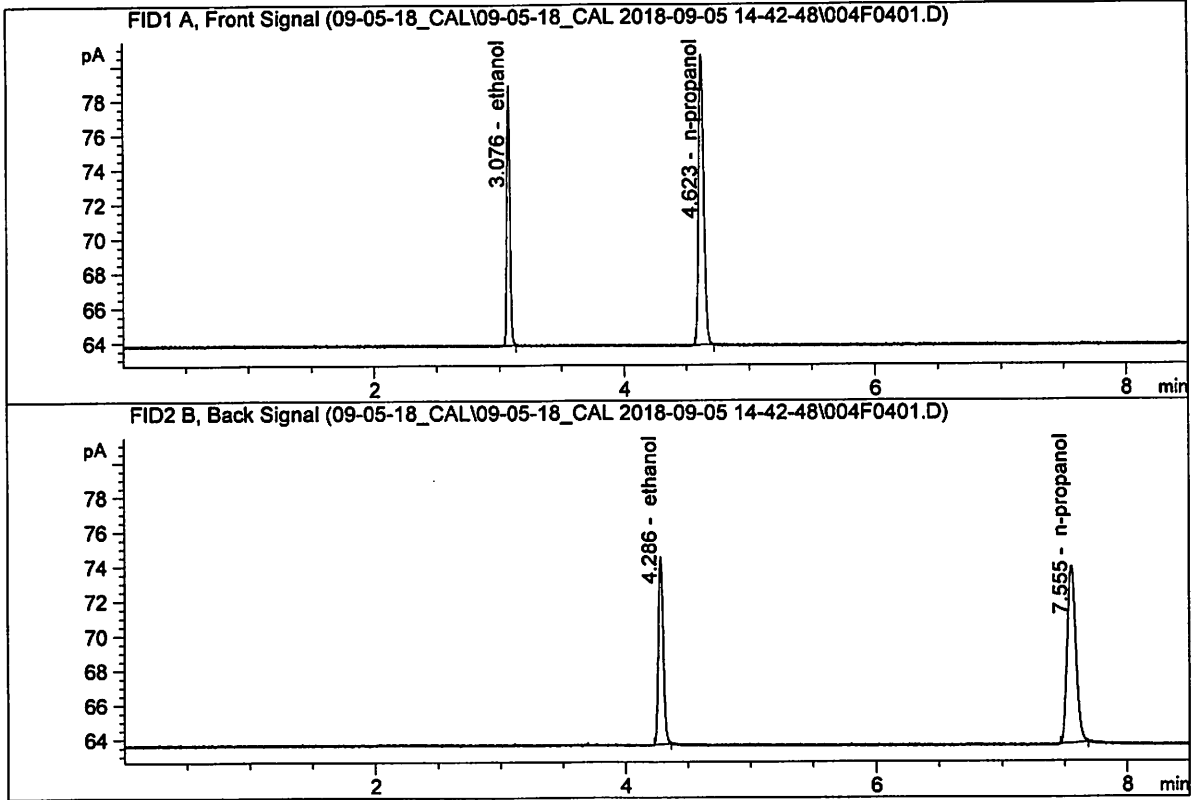

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	27.45264	0.3008	g/100cc
2.	Ethanol	Column 2:	28.79560	0.3002	g/100cc
3.	n-Propanol	Column 1:	47.70254	1.0000	g/100cc
4.	n-Propanol	Column 2:	49.17295	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.500 FN07031402  
 Laboratory : Meridian  
 Injection Date : Sep 5, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

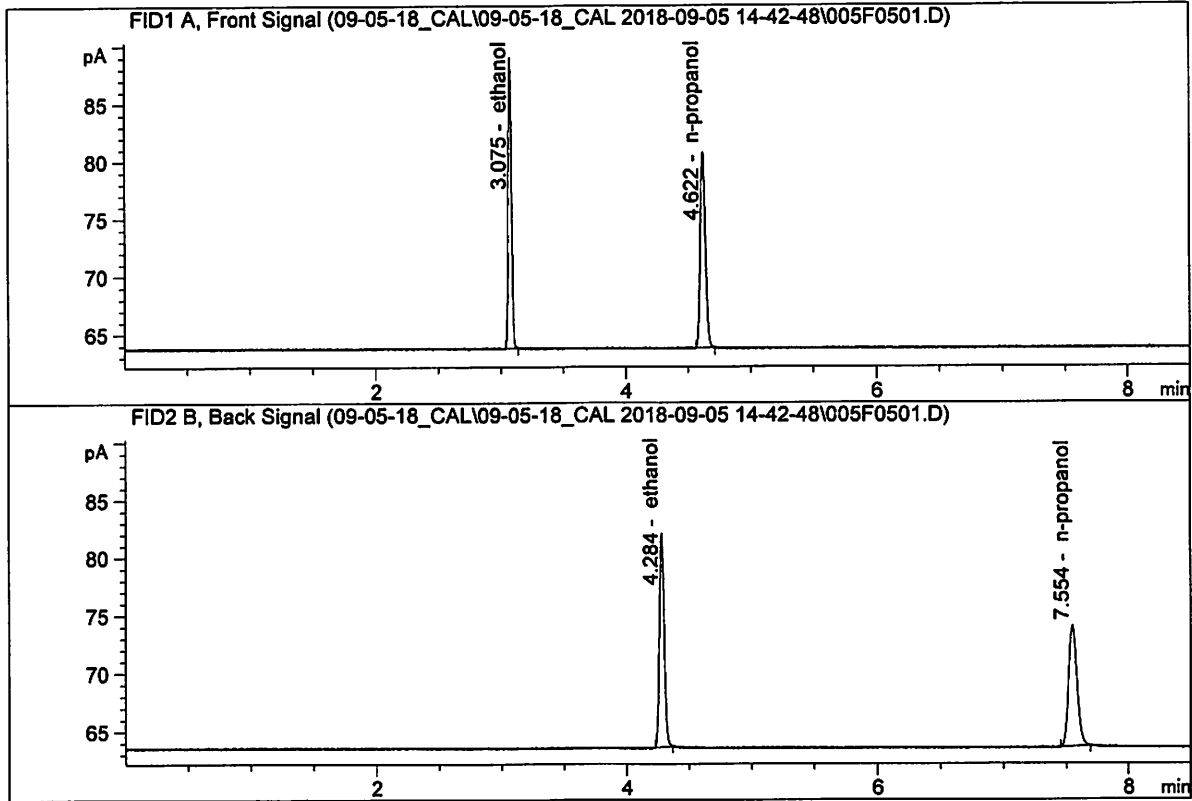


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	46.08223	0.4997	g/100cc
2.	Ethanol	Column 2:	48.70642	0.5003	g/100cc
3.	n-Propanol	Column 1:	48.15673	1.0000	g/100cc
4.	n-Propanol	Column 2:	49.65463	1.0000	g/100cc

66

ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STANDARD BLANK  
 Laboratory : Meridian  
 Injection Date : Sep 5, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

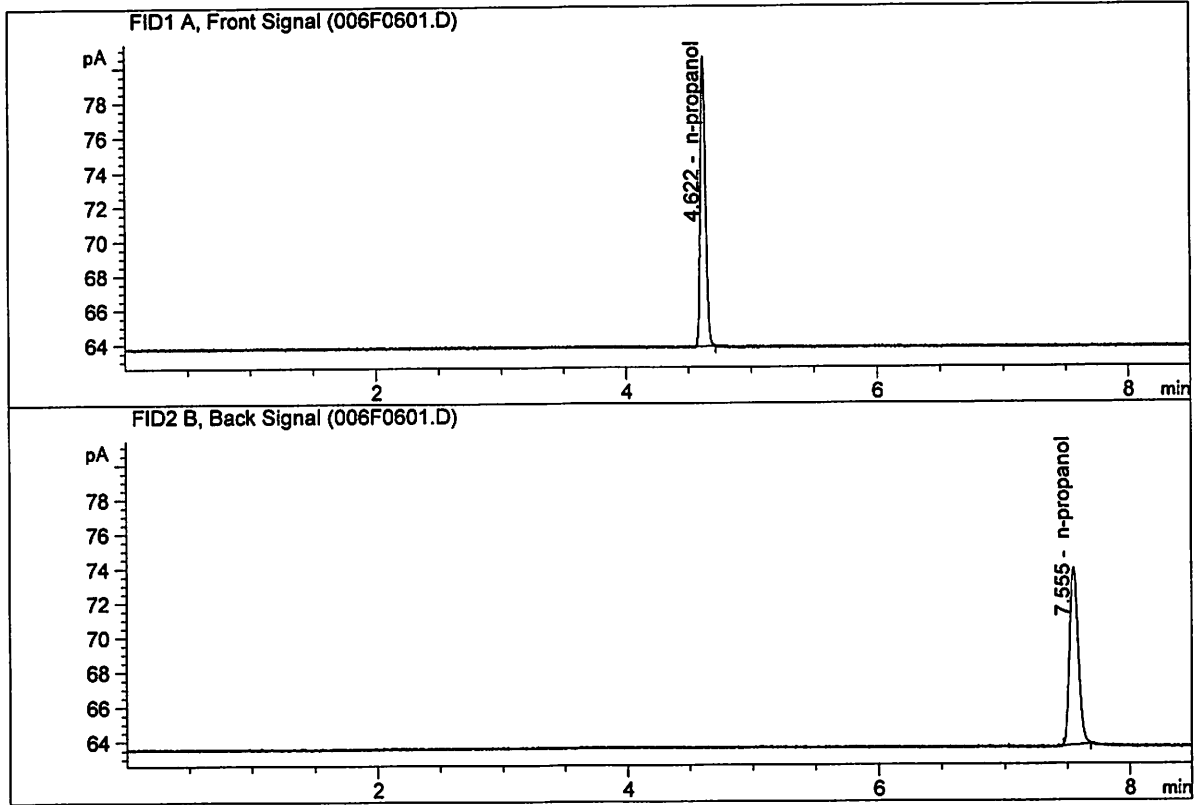

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	47.67532	1.0000	g/100cc
4.	n-Propanol	Column 2:	48.94547	1.0000	g/100cc

S a m p l e S u m m a r y


Sequence table: C:\Chem32\1\Data\09-05-18\_CAL\09-05-18\_CAL 2018-09-05 14-42-48\09-05-18\_CAL.S  
 Data directory path: C:\Chem32\1\Data\09-05-18\_CAL\09-05-18\_CAL 2018-09-05 14-42-48\  
 Logbook: C:\Chem32\1\Data\09-05-18\_CAL\09-05-18\_CAL 2018-09-05 14-42-48\09-05-18\_CAL.LOG  
 Sequence start: 9/5/2018 2:57:23 PM  
 Sequence Operator: SYSTEM  
 Operator: SYSTEM  
 Method file name: C:\Chem32\1\Data\09-05-18\_CAL\09-05-18\_CAL 2018-09-05 14-42-48\ALCOHOL.M

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #	Cmp
1	1	1	0.050 FN06231406	-	1.0000	001F0101.D	*	4
2	2	1	0.100 FN08101601	-	1.0000	002F0201.D	*	4
3	3	1	0.200 FN12011401	-	1.0000	003F0301.D	*	4
4	4	1	0.300 FN02121601	-	1.0000	004F0401.D	*	4
5	5	1	0.500 FN07031402	-	1.0000	005F0501.D	*	4
6	6	1	INTERNAL STANDAR	-	1.0000	006F0601.D		2

JK

ISP Forensic Services Blood Alcohol Report


Sample Name : INTERNAL STD BLK 1  
 Laboratory : Meridian  
 Injection Date : Sep 5, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

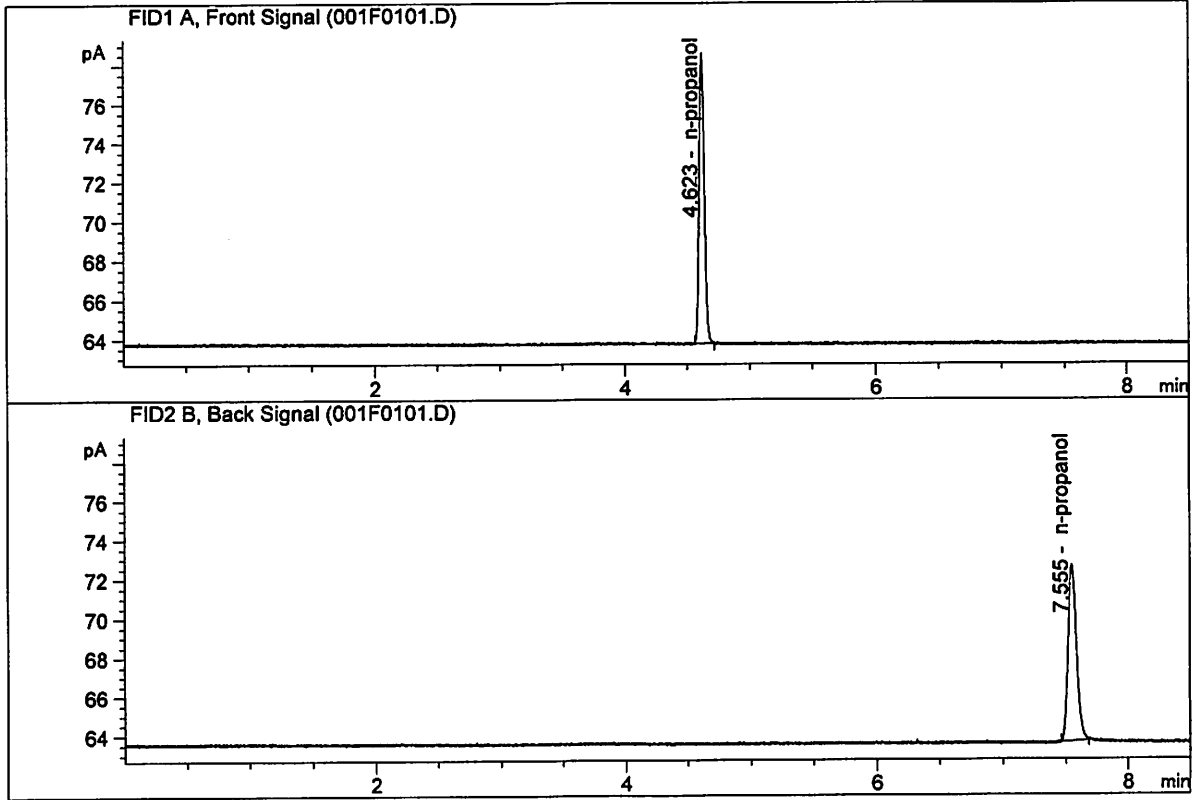

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	42.21704	1.0000	g/100cc
4.	n-Propanol	Column 2:	43.39153	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report

Sample Name : MIX VOL FN06041502  
 Laboratory : Meridian  
 Injection Date : Sep 5, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

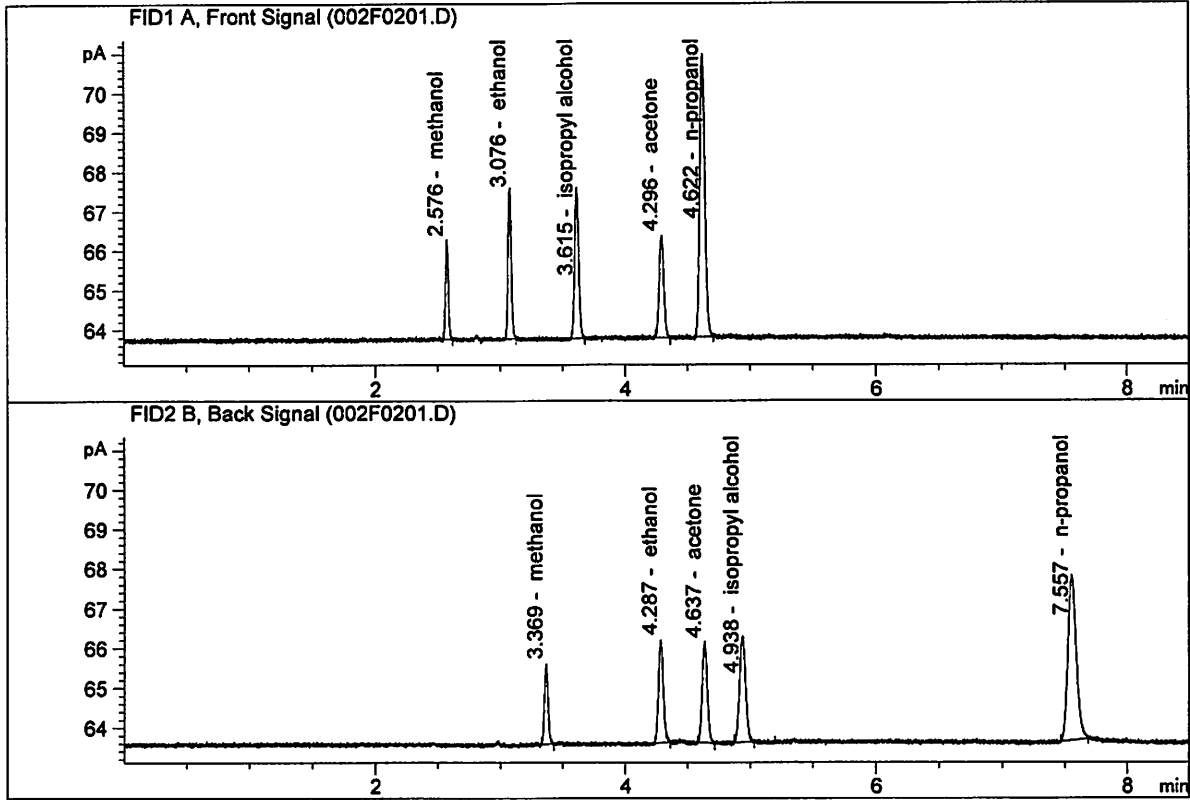

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	6.69122	0.1741	g/100cc
2.	Ethanol	Column 2:	6.92505	0.1791	g/100cc
3.	n-Propanol	Column 1:	20.12340	1.0000	g/100cc
4.	n-Propanol	Column 2:	19.99166	1.0000	g/100cc



## VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC1-1

Analysis Date(s): 05 Sep 2018

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.0785	0.0794	0.0009	0.0789	0.0793	
(g/100cc)	0.0793	0.0800	0.0007	0.0796		

### Analysis Method

Refer to Blood Alcohol Method #1

### Instrument Information

*Instrument method is stored centrally.*

Refer to Instrument Method: ALCOHOL.M  
Hamilton Auto-Dilutor Serial Number: ML600HC11378

### Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.079	0.075	0.083	0.004

	<b>Reported Result</b> <hr style="border-top: 1px dashed black;"/> <p style="text-align: center; margin: 0;">0.079</p>	
--	---	--

*Calibration and control data are stored centrally.*


Issued: 12/30/2016

Volatiles BAC Calculation Spreadsheet Rev 4

Issuing Authority: Quality Manager

ISP Forensic Services Blood Alcohol Report


Sample Name : QC1-1-A  
 Laboratory : Meridian  
 Injection Date : Sep 5, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

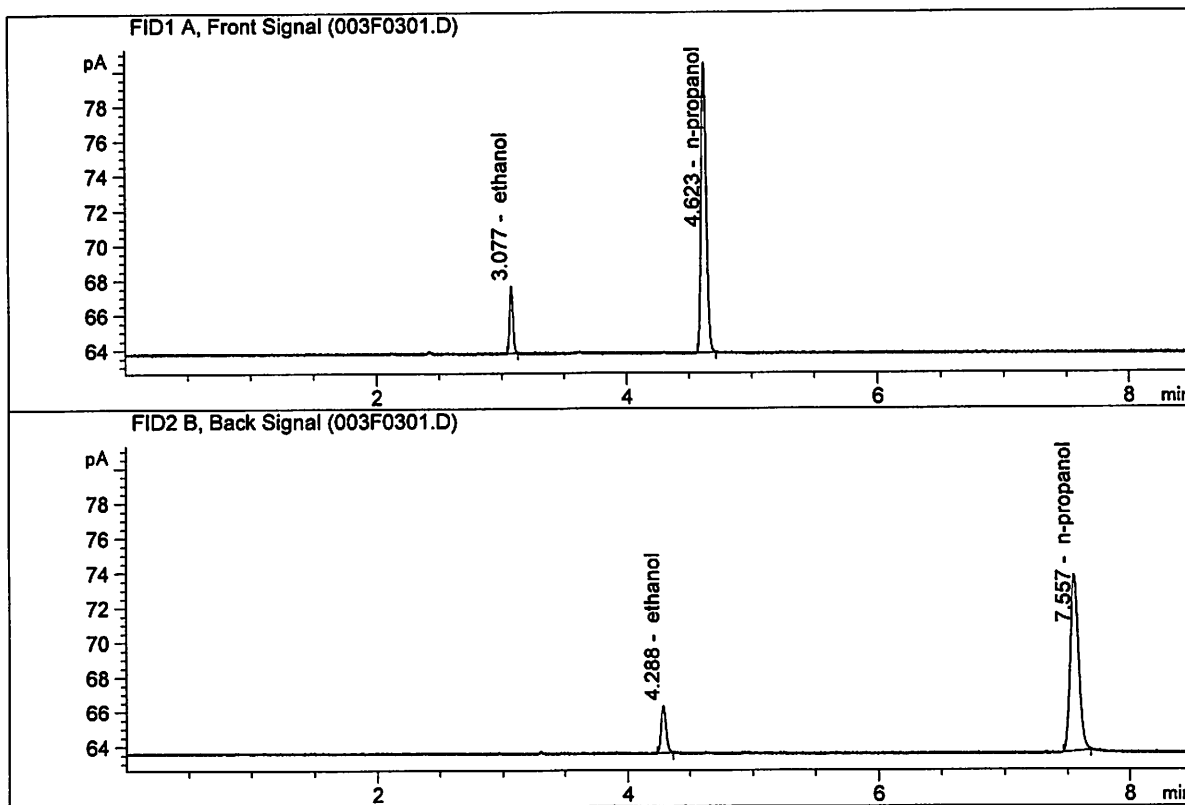

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.08311	0.0785	g/100cc
2.	Ethanol	Column 2:	7.25821	0.0794	g/100cc
3.	n-Propanol	Column 1:	47.43428	1.0000	g/100cc
4.	n-Propanol	Column 2:	48.57603	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-1-B  
 Laboratory : Meridian  
 Injection Date : Sep 5, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

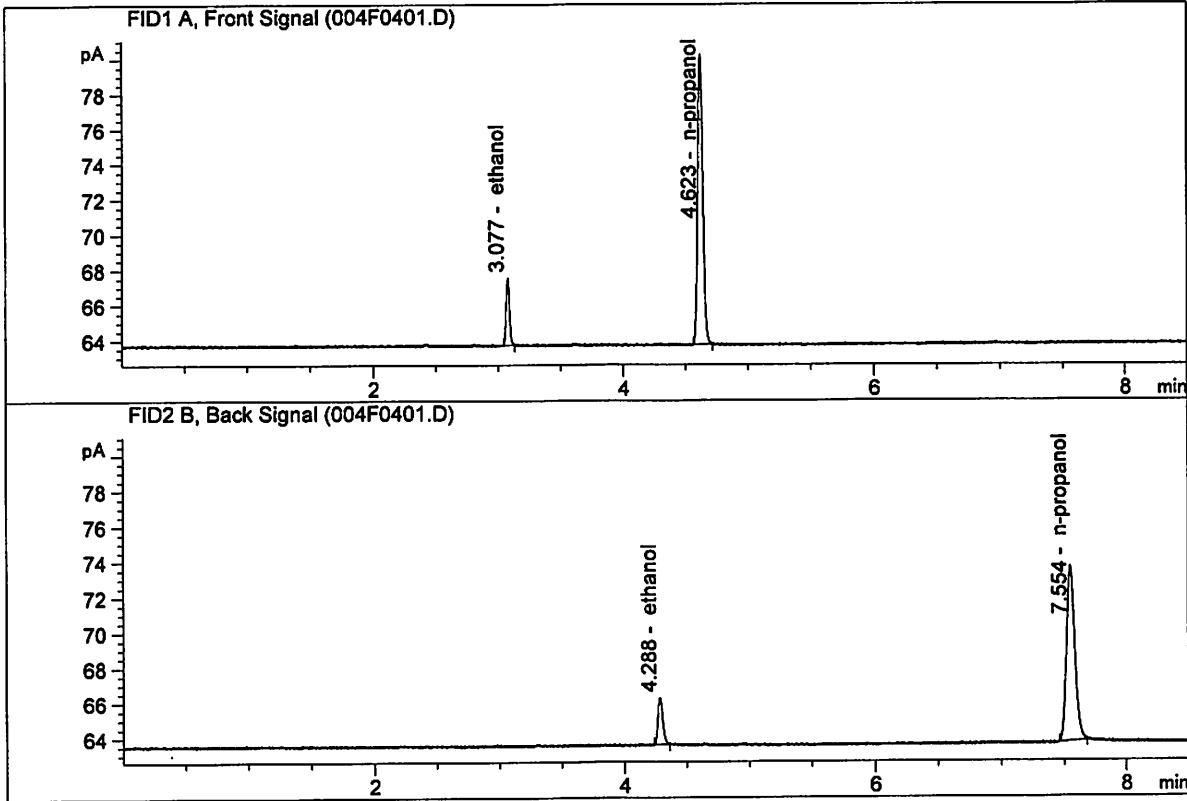

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.07998	0.0793	g/100cc
2.	Ethanol	Column 2:	7.22853	0.0800	g/100cc
3.	n-Propanol	Column 1:	46.95176	1.0000	g/100cc
4.	n-Propanol	Column 2:	48.01218	1.0000	g/100cc

JK

## VOLATILES DETERMINATION CASEFILE WORKSHEET

**Laboratory No.: 0.08 FN04171701**

**Analysis Date(s): 05 Sep 2018**

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.0796	0.0804	0.0008	0.0800	0.0805	
(g/100cc)	0.0806	0.0814	0.0008	0.0810		

**Analysis Method**

Refer to Blood Alcohol Method #1

**Instrument Information**

*Instrument method is stored centrally.*

Refer to Instrument Method: ALCOHOL.M  
Hamilton Auto-Dilutor Serial Number: ML600HC11378

**Reporting of Results**

**Uncertainty of Measurement (UM%): 5.00%**

Overall Mean (g/100cc)	Low	High	5% of Mean
0.080	0.076	0.084	0.004

	<b>Reported Result</b>  0.080	
--	-------------------------------------	--

*Calibration and control data are stored centrally.*

Issued: 12/30/2016


Volatiles BAC Calculation Spreadsheet Rev 4

Issuing Authority: Quality Manager

JK

ISP Forensic Services Blood Alcohol Report


Sample Name : 0.08 FN04171701-A  
 Laboratory : Meridian  
 Injection Date : Sep 5, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

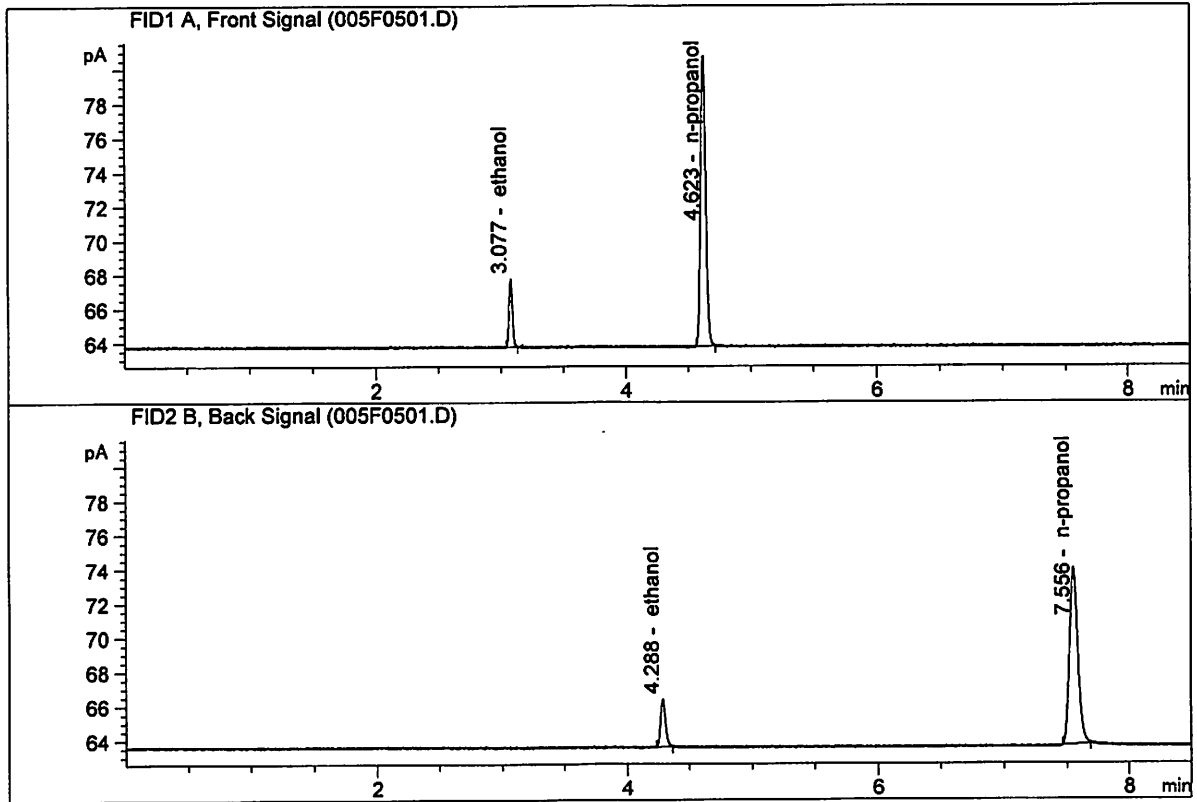

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.31988	0.0796	g/100cc
2.	Ethanol	Column 2:	7.49614	0.0804	g/100cc
3.	n-Propanol	Column 1:	48.33976	1.0000	g/100cc
4.	n-Propanol	Column 2:	49.54201	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.08 FN04171701-B  
 Laboratory : Meridian  
 Injection Date : Sep 5, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

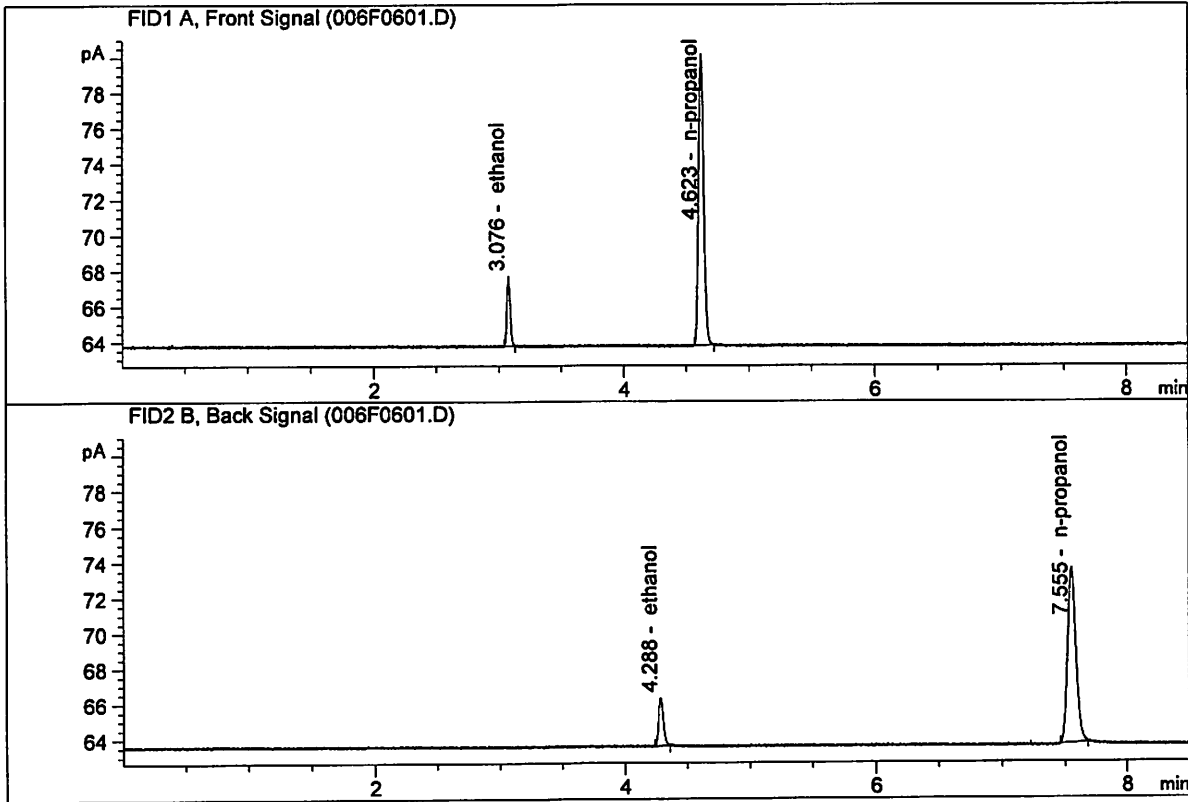

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.15636	0.0806	g/100cc
2.	Ethanol	Column 2:	7.31731	0.0814	g/100cc
3.	n-Propanol	Column 1:	46.69572	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.72866	1.0000	g/100cc

## VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC2-1

Analysis Date(s): 05 Sep 2018

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.2000	0.2015	0.0015	0.2007	0.2011	
(g/100cc)	0.2012	0.2019	0.0007	0.2015		

**Analysis Method**

Refer to Blood Alcohol Method #1

**Instrument Information**

*Instrument method is stored centrally.*

Refer to Instrument Method: ALCOHOL.M  
Hamilton Auto-Dilutor Serial Number: ML600HC11378

**Reporting of Results**

**Uncertainty of Measurement (UM%): 5.00%**

Overall Mean (g/100cc)	Low	High	5% of Mean
0.201	0.190	0.212	0.011


	<b>Reported Result</b>	
	0.201	

*Calibration and control data are stored centrally.*

86

ISP Forensic Services Blood Alcohol Report

Sample Name : QC2-1-A  
 Laboratory : Meridian  
 Injection Date : Sep 5, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

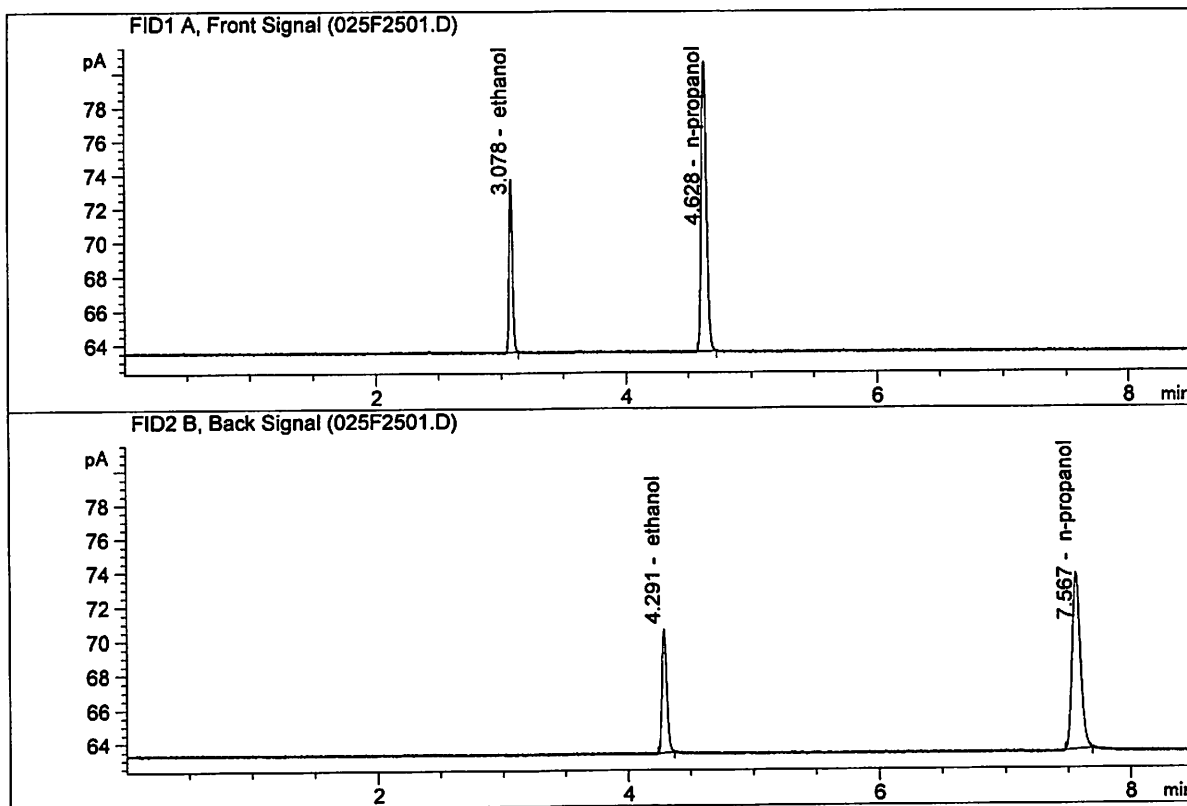


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	18.60257	0.2000	g/100cc
2.	Ethanol	Column 2:	19.38306	0.2015	g/100cc
3.	n-Propanol	Column 1:	48.67100	1.0000	g/100cc
4.	n-Propanol	Column 2:	49.61661	1.0000	g/100cc



ISP Forensic Services Blood Alcohol Report

Sample Name : QC2-1-B  
 Laboratory : Meridian  
 Injection Date : Sep 5, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

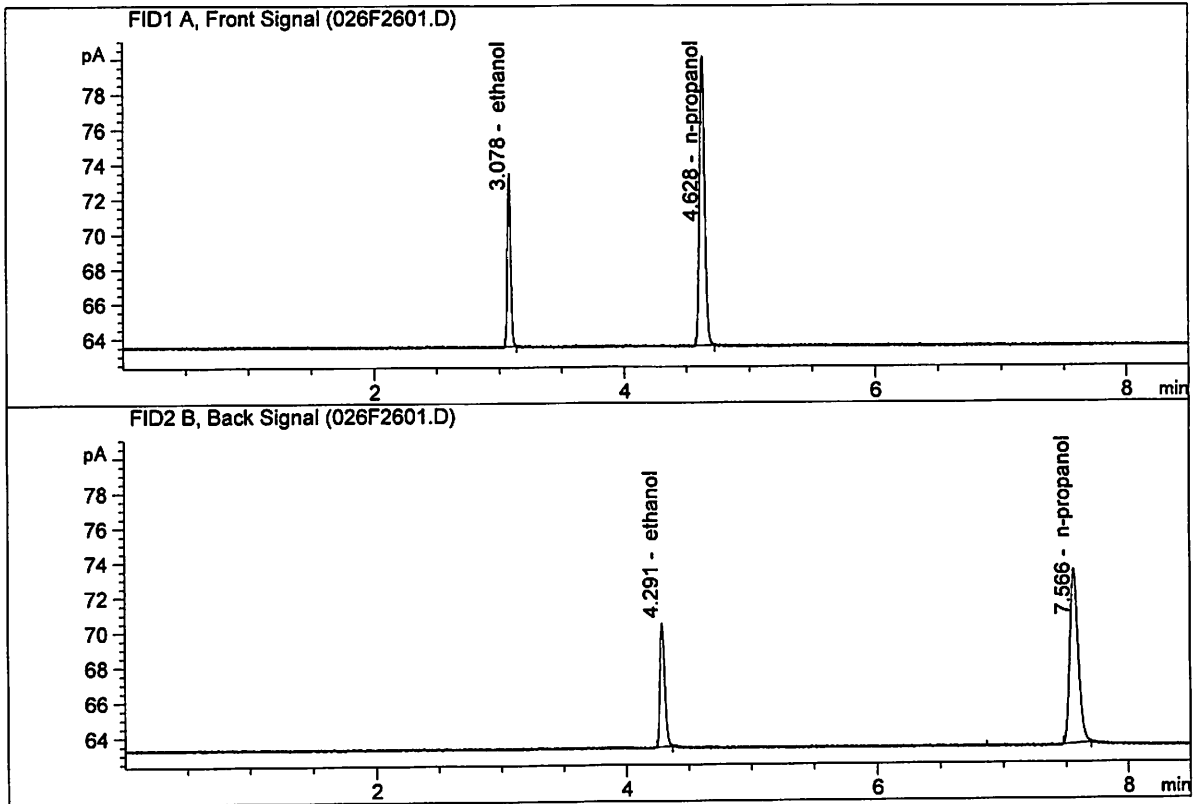

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	18.21739	0.2012	g/100cc
2.	Ethanol	Column 2:	18.87497	0.2019	g/100cc
3.	n-Propanol	Column 1:	47.38148	1.0000	g/100cc
4.	n-Propanol	Column 2:	48.23109	1.0000	g/100cc

## VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC1-2

Analysis Date(s): 06 Sep 2018

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.0828	0.0837	0.0009	0.0832	0.0827	
(g/100cc)	0.0816	0.0827	0.0011	0.0821		

**Analysis Method**

Refer to Blood Alcohol Method #1

**Instrument Information**

*Instrument method is stored centrally.*

Refer to Instrument Method: ALCOHOL.M  
Hamilton Auto-Dilutor Serial Number: ML600HC11378

**Reporting of Results**

**Uncertainty of Measurement (UM%): 5.00%**


Overall Mean (g/100cc)	Low	High	5% of Mean
0.082	0.077	0.087	0.005

	<b>Reported Result</b>  0.082	
--	-------------------------------------	--

*Calibration and control data are stored centrally.*

ISP Forensic Services Blood Alcohol Report


Sample Name : QC1-2-A  
 Laboratory : Meridian  
 Injection Date : Sep 6, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014 - CN11041167

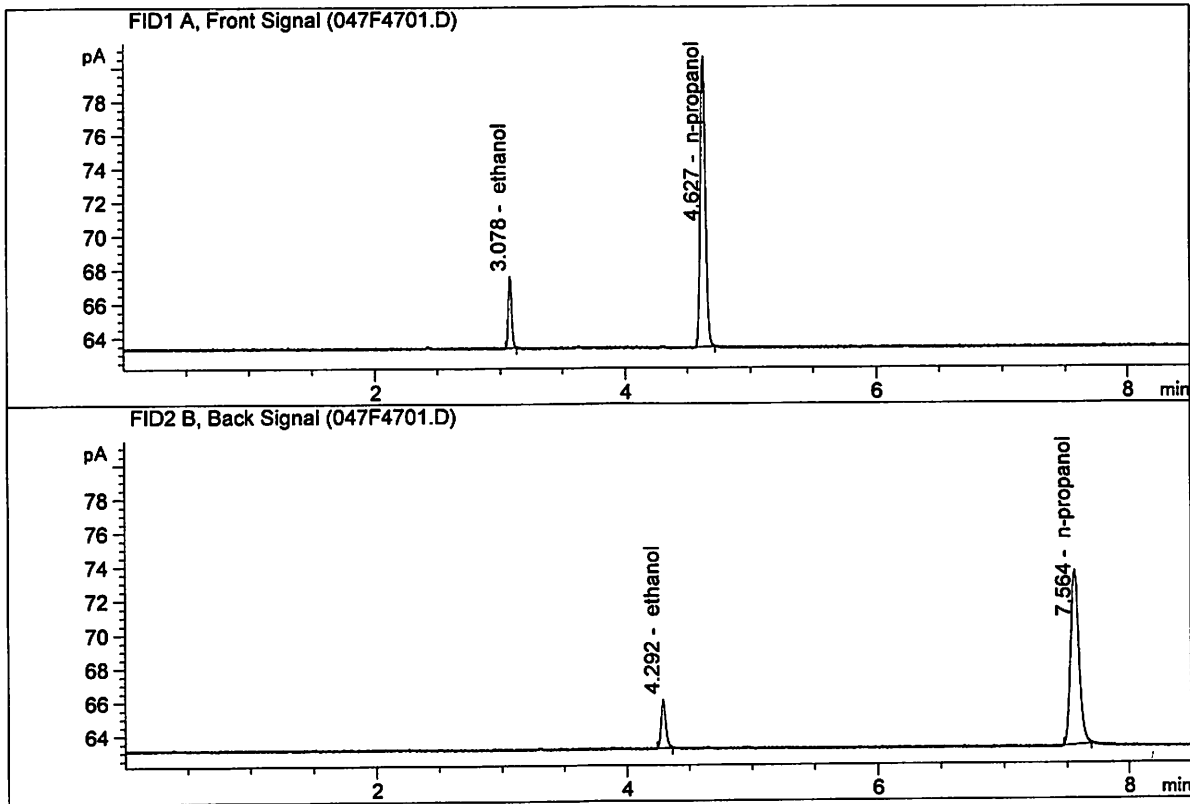

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.67254	0.0828	g/100cc
2.	Ethanol	Column 2:	7.86928	0.0837	g/100cc
3.	n-Propanol	Column 1:	48.72801	1.0000	g/100cc
4.	n-Propanol	Column 2:	49.84349	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report


Sample Name : QC1-2-B  
 Laboratory : Meridian  
 Injection Date : Sep 6, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

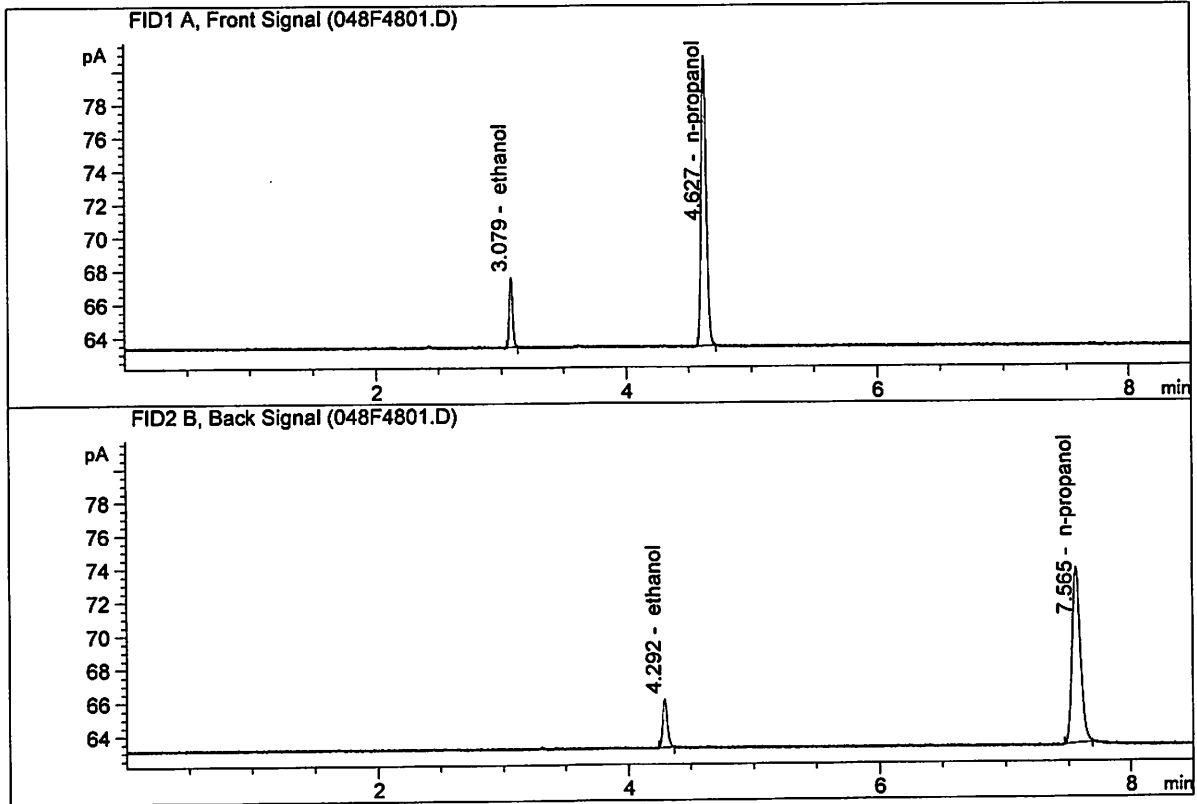

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.67915	0.0816	g/100cc
2.	Ethanol	Column 2:	7.87194	0.0827	g/100cc
3.	n-Propanol	Column 1:	49.45396	1.0000	g/100cc
4.	n-Propanol	Column 2:	50.51962	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STD BLK  
 Laboratory : Meridian  
 Injection Date : Sep 6, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

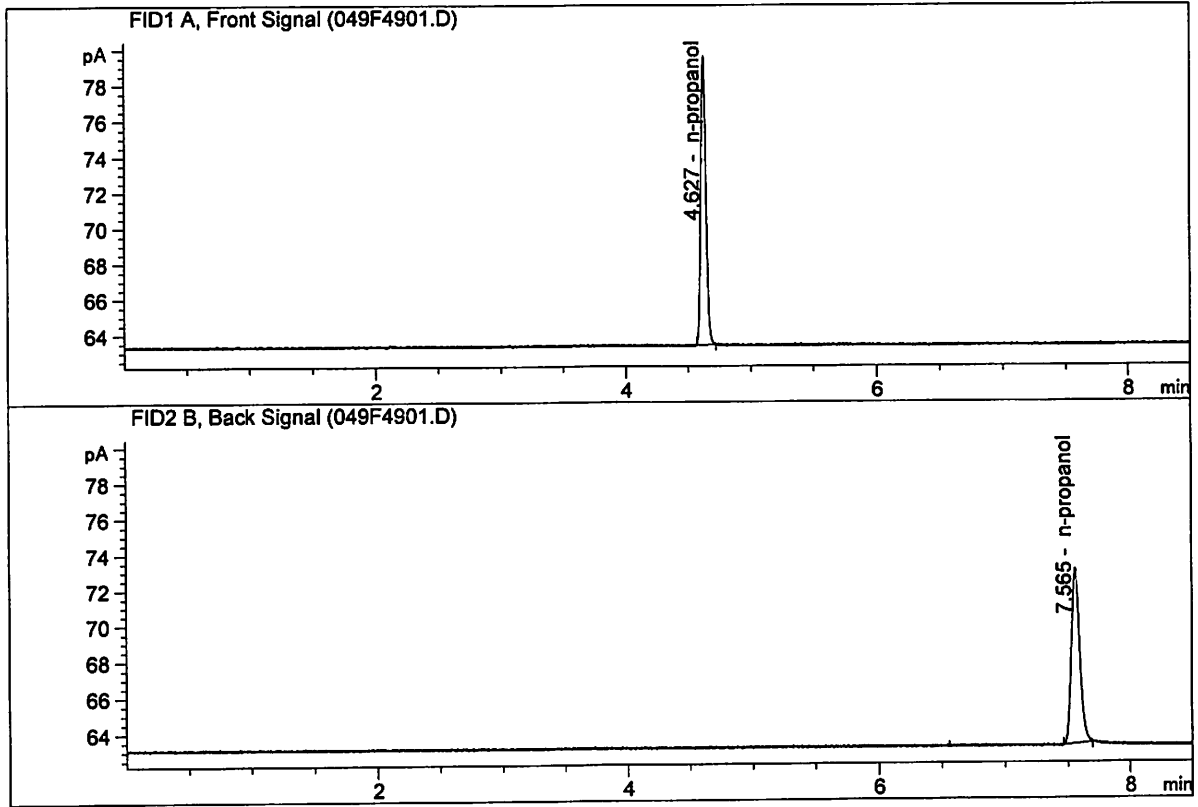

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	46.20098	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.19557	1.0000	g/100cc

S a m p l e S u m m a r y

Sequence table: C:\Chem32\1\Data\09-05-18\_SAMPLES\09-05-18\_SAMPLES 2018-09-05 16-09-17\09-05-18\_SAMPLES.S  
 Data directory path: C:\Chem32\1\Data\09-05-18\_SAMPLES\09-05-18\_SAMPLES 2018-09-05 16-09-17\  
 Logbook: C:\Chem32\1\Data\09-05-18\_SAMPLES\09-05-18\_SAMPLES 2018-09-05 16-09-17\09-05-18\_SAMPLES.LOG  
 Sequence start: 9/5/2018 4:24:02 PM  
 Sequence Operator: SYSTEM  
 Operator: SYSTEM  
 Method file name: C:\Chem32\1\Data\09-05-18\_SAMPLES\09-05-18\_SAMPLES 2018-09-05 16-09-17\ALCOHOL.M

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #	# Cmp
1	1	1	INTERNAL STD BLK	-	1.0000	001F0101.D		2
2	2	1	MIX VOL FN060415	-	1.0000	002F0201.D		10
3	3	1	QC1-1-A	-	1.0000	003F0301.D		4
4	4	1	QC1-1-B	-	1.0000	004F0401.D		4
5	5	1	0.08 FN04171701-	-	1.0000	005F0501.D		4
6	6	1	0.08 FN04171701-	-	1.0000	006F0601.D		4
7	7	1	M2018-4314-1-A	-	1.0000	007F0701.D		4
8	8	1	M2018-4314-1-B	-	1.0000	008F0801.D		4
9	9	1	M2018-4316-1-A	-	1.0000	009F0901.D		6
10	10	1	M2018-4316-1-B	-	1.0000	010F1001.D		6
11	11	1	M2018-4317-1-A	-	1.0000	011F1101.D		2
12	12	1	M2018-4317-1-B	-	1.0000	012F1201.D		2
13	13	1	M2018-4324-3-A	-	1.0000	013F1301.D		4
14	14	1	M2018-4324-3-B	-	1.0000	014F1401.D		4
15	15	1	M2018-4324-4-A	-	1.0000	015F1501.D		2
16	16	1	M2018-4324-4-B	-	1.0000	016F1601.D		2
17	17	1	M2018-4330-1-A	-	1.0000	017F1701.D		2
18	18	1	M2018-4330-1-B	-	1.0000	018F1801.D		2
19	19	1	M2018-4330-2-A	-	1.0000	019F1901.D		2
20	20	1	M2018-4330-2-B	-	1.0000	020F2001.D		2
21	21	1	M2018-4331-1-A	-	1.0000	021F2101.D		2
22	22	1	M2018-4331-1-B	-	1.0000	022F2201.D		2
23	23	1	M2018-4332-1-A	-	1.0000	023F2301.D		6
24	24	1	M2018-4332-1-B	-	1.0000	024F2401.D		6
25	25	1	QC2-1-A	-	1.0000	025F2501.D		4
26	26	1	QC2-1-B	-	1.0000	026F2601.D		4
27	27	1	M2018-4346-1-A	-	1.0000	027F2701.D		4
28	28	1	M2018-4346-1-B	-	1.0000	028F2801.D		4
29	29	1	M2018-4347-1-A	-	1.0000	029F2901.D		4
30	30	1	M2018-4347-1-B	-	1.0000	030F3001.D		4
31	31	1	M2018-4348-1-A	-	1.0000	031F3101.D		2
32	32	1	M2018-4348-1-B	-	1.0000	032F3201.D		2
33	33	1	M2018-4370-1-A	-	1.0000	033F3301.D		4
34	34	1	M2018-4370-1-B	-	1.0000	034F3401.D		4
35	35	1	M2018-4375-1-A	-	1.0000	035F3501.D		4
36	36	1	M2018-4375-1-B	-	1.0000	036F3601.D		4
37	37	1	M2018-4376-1-A	-	1.0000	037F3701.D		4
38	38	1	M2018-4376-1-B	-	1.0000	038F3801.D		4
39	39	1	M2018-4378-1-A	-	1.0000	039F3901.D		6
40	40	1	M2018-4378-1-B	-	1.0000	040F4001.D		6
41	41	1	M2018-4379-1-A	-	1.0000	041F4101.D		6
42	42	1	M2018-4379-1-B	-	1.0000	042F4201.D		6
43	43	1	M2018-4387-1-A	-	1.0000	043F4301.D		4

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #	# Cmp
44	44	1	M2018-4387-1-B	-	1.0000	044F4401.D		4
45	45	1	M2018-4411-1-A	-	1.0000	045F4501.D		4
46	46	1	M2018-4411-1-B	-	1.0000	046F4601.D		4
47	47	1	QC1-2-A	-	1.0000	047F4701.D		4
48	48	1	QC1-2-B	-	1.0000	048F4801.D		4
49	49	1	INTERNAL STD BLK	-	1.0000	049F4901.D		2

Method file name: C:\Chem32\1\Data\09-05-18\_SAMPLES\09-05-18\_SAMPLES 2018-09-05 16-09-17  
 \SHUTDOWN.M

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #	# Cmp
50	50	1	EMPTY	-	1.0000	050F5001.D		0