


















Worklist: 3983

<u>LAB CASE</u>	<u>ITEM</u>	<u>ITEM TYPE</u>	<u>DESCRIPTION</u>	
M2020-0306	2	BCK	Alcohol Analysis	
M2020-0322	1	BCK	Alcohol Analysis	
M2020-0323	1	BCK	Alcohol Analysis	
M2020-0343	1	BCK	Alcohol Analysis	
M2020-0344	1	BCK	Alcohol Analysis	
M2020-0358	2	BCK	Alcohol Analysis	
M2020-0359	1	BCK	Alcohol Analysis	
M2020-0362	1	BCK	Alcohol Analysis	
M2020-0377	1	BCK	Alcohol Analysis	
M2020-0415	1	BCK	Alcohol Analysis	
M2020-0416	1	BCK	Alcohol Analysis	
M2020-0424	2	BCK	Alcohol Analysis	
M2020-0448	1	UCK	Alcohol Analysis	
M2020-0448	2	BCK	Alcohol Analysis	
M2020-0476	1	BCK	Alcohol Analysis	
M2020-0477	1	BCK	Alcohol Analysis	
M2020-0478	1	BCK	Alcohol Analysis	
M2020-0479	1	BCK	Alcohol Analysis	

REVIEWED
By Jeremy Johnston at 10:00 am, Feb 06, 2020



Quantitative Analysis for Ethanol & Qualitative Analysis for Other Volatiles

Analytical Method(s): 1.0

Device: Hamilton MICROLAB Liquid Processor/Dilutor Serial Number: ML600HC11378

Volatiles Quality Assurance Controls Run Date(s): 02/05/2020

Calibration Date: 02/05/2020

Control level	Expiration	Lot #	Target Value	Acceptable Range	Overall Results
Level 1	Jan-22	1801036	0.0812	0.0731-0.0893	0.0789 g/100cc 0.0806 g/100cc g/100cc
Level 2	Mar-22	1803028	0.2035	0.1832-0.2238	0.1954 g/100cc g/100cc
Multi-Component mixture:			Lot #	FN06041502	OK
Curve Fit:			Column 1	1.00000	Column2
					0.99994

Ethanol Calibration Reference Material

Calibrator level	Target Value	Acceptable Range	Column 1	Column 2	Precision	Mean
50	0.050	0.045 - 0.055	0.0504	0.0518	0.0014	0.0511
100	0.100	0.090 - 0.110	0.0997	0.1005	0.0008	0.1001
200	0.200	0.180 - 0.220	0.2001	0.1980	0.0021	0.199
300	0.300	0.270 - 0.330	0.2994	0.2980	0.0014	0.2987
400	0.400	0.360 - 0.440				
500	0.500	0.450 - 0.550	0.5003	0.5017	0.0014	0.501

Aqueous Controls

Control level	Target Value	Acceptable Range	Overall Results
80	0.080	0.076 - 0.084	0.080 g/100cc

=====
Calibration Table
=====

General Calibration Setting

Calib. Data Modified : Wednesday, February 05, 2020 9:40:43 AM
Signals calculated separately : No

Rel. Reference Window : 0.000 %
Abs. Reference Window : 0.100 min
Rel. Non-ref. Window : 0.000 %
Abs. Non-ref. Window : 0.100 min
Uncalibrated Peaks : not reported
Partial Calibration : Yes, identified peaks are recalibrated
Correct All Ret. Times: No, only for identified peaks

Curve Type : Linear
Origin : Ignored
Weight : Equal

Recalibration Settings:
Average Response : Average all calibrations
Average Retention Time: Floating Average New 75%

Calibration Report Options :
Printout of recalibrations within a sequence:
Calibration Table after Recalibration
Normal Report after Recalibration
If the sequence is done with bracketing:
Results of first cycle (ending previous bracket)

Default Sample ISTD Information (if not set in sample table):

ISTD #	ISTD Amount [g/100cc]	Name
1	1.00000	n-propanol
2	1.00000	n-propanol

Signal Details

Signal 1: FID1 A, Front Signal
Signal 2: FID2 B, Back Signal

Overview Table

RT	Sig	Lvl	Amount [g/100cc]	Area	Rsp.Factor	Ref	ISTD #	Compound
2.586	1	1	1.00000	3.69669	2.70512e-1	No	No 1	methanol
2.809	1	1	1.00000	4.26100	2.34687e-1	No	No 2	Acetaldehyde
2.977	2	1	1.00000	4.26100	2.34687e-1	No	No 2	Acetaldehyde
3.075	1	1	5.00000e-2	4.52242	1.10560e-2	No	No 1	ethanol
			1.00000e-1	9.04952	1.10503e-2			
			2.00000e-1	18.19493	1.09921e-2			
			3.00000e-1	27.40895	1.09453e-2			
			5.00000e-1	45.87756	1.08986e-2			
3.388	2	1	1.00000	4.26062	2.34707e-1	No	No 2	methanol
3.628	1	1	1.00000	9.73055	1.02769e-1	No	No 1	isopropyl alcohol
4.285	2	1	5.00000e-2	4.62532	1.08101e-2	No	No 2	ethanol
			1.00000e-1	9.39700	1.06417e-2			
			2.00000e-1	18.84535	1.06127e-2			
			3.00000e-1	28.70562	1.04509e-2			
			5.00000e-1	48.52429	1.03041e-2			
4.308	1	1	1.00000	6.49940	1.53860e-1	No	No 1	acetone
4.620	1	1	1.00000	44.08209	2.26850e-2	No	Yes 1	n-propanol
			1.00000	44.16013	2.26449e-2			
			1.00000	44.01959	2.27172e-2			
			1.00000	44.24614	2.26008e-2			
			1.00000	44.25955	2.25940e-2			
4.661	2	1	1.00000	6.89301	1.45075e-1	No	No 2	acetone
4.969	2	1	1.00000	10.70642	9.34019e-2	No	No 2	isopropyl alcohol
7.550	2	1	1.00000	45.86525	2.18030e-2	No	Yes 2	n-propanol
			1.00000	45.63153	2.19147e-2			
			1.00000	45.28697	2.20814e-2			
			1.00000	45.42099	2.20163e-2			
			1.00000	45.29530	2.20773e-2			


Peak Sum Table

No Entries in table

1 Warnings or Errors :


Warning : Curve requires more calibration points., (methanol)

Calibration Curves

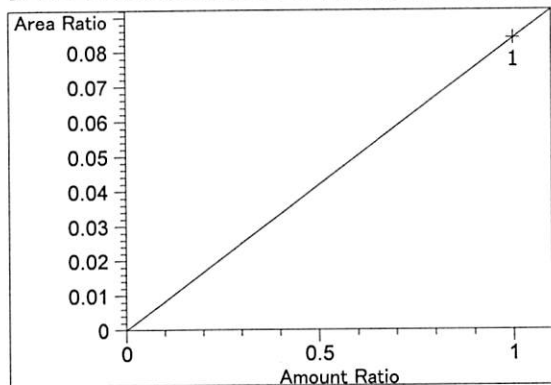


methanol at exp. RT: 2.586
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 8.38593e-2
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio


W

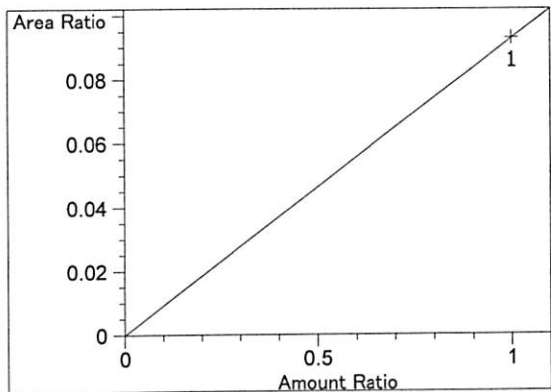


Acetaldehyde at exp. RT: 2.809
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 9.29026e-2
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio

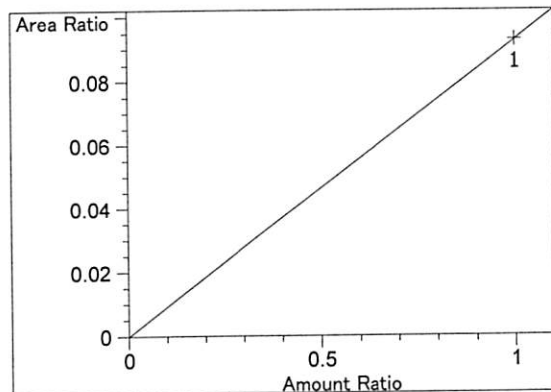

Acetaldehyde at exp. RT: 2.977
 FID2 B, Back Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 9.29026e-2
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio

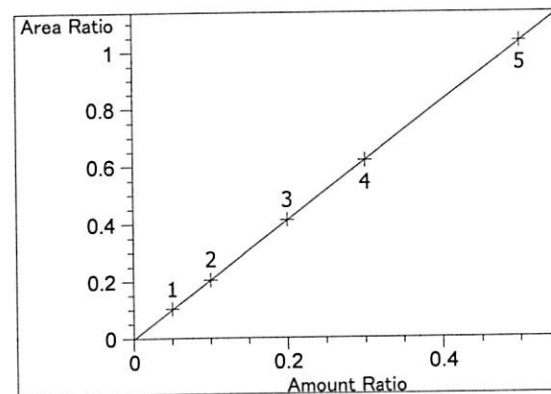


ethanol at exp. RT: 3.075
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00102
 Formula: $y = mx + b$
 m: 2.07599
 b: -2.10191e-3
 x: Amount Ratio
 y: Area Ratio

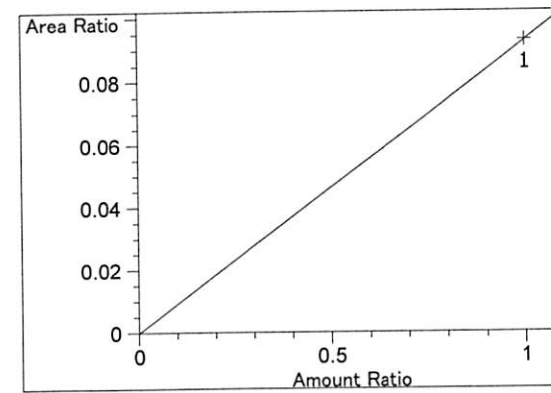


methanol at exp. RT: 3.388
 FID2 B, Back Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 9.28944e-2
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio


W

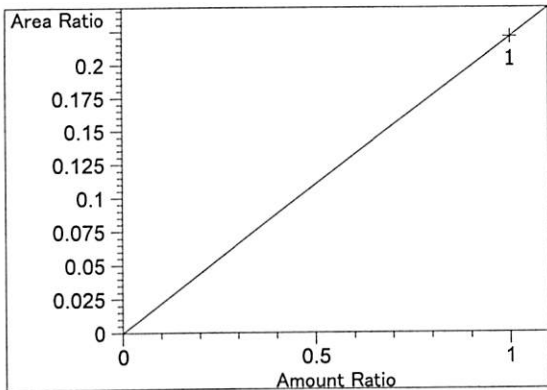


isopropyl alcohol at exp. RT: 3.628
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 2.20737e-1
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio

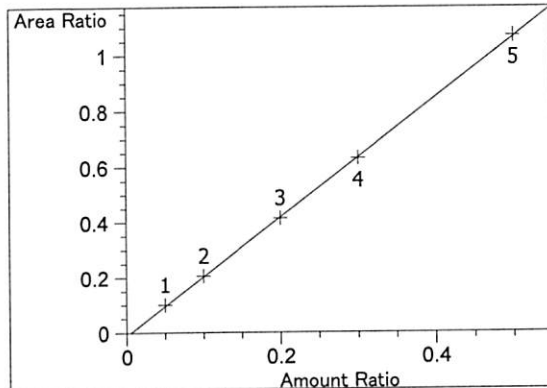

ethanol at exp. RT: 4.285
 FID2 B, Back Signal
 Correlation: 0.99994
 Residual Std. Dev.: 0.00472
 Formula: $y = mx + b$
 m: 2.15687
 b: -1.08430e-2
 x: Amount Ratio
 y: Area Ratio

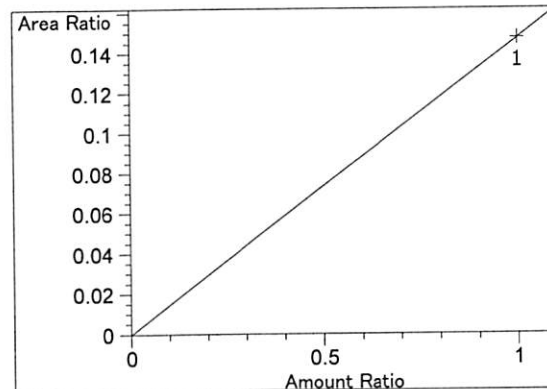


acetone at exp. RT: 4.308
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 1.47439e-1
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio

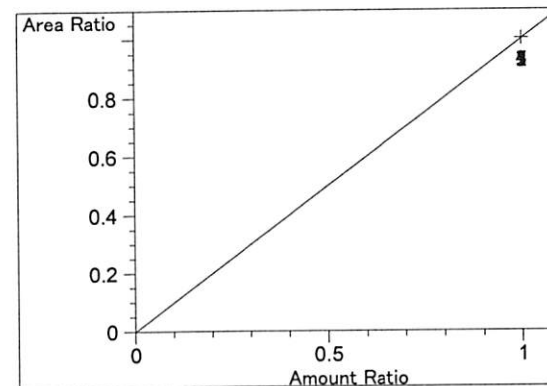


n-propanol at exp. RT: 4.620
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 1.00000
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio


W

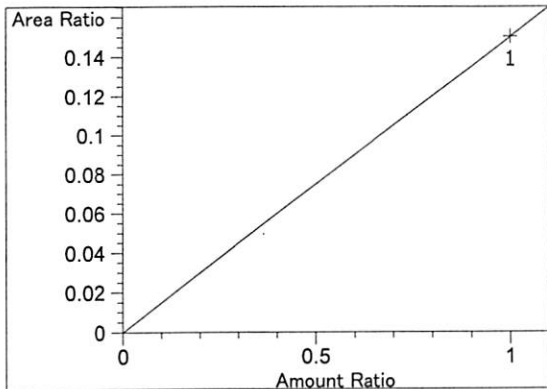

acetone at exp. RT: 4.661
FID2 B, Back Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx + b$
m: 1.50288e-1
b: 0.00000
x: Amount Ratio
y: Area Ratio

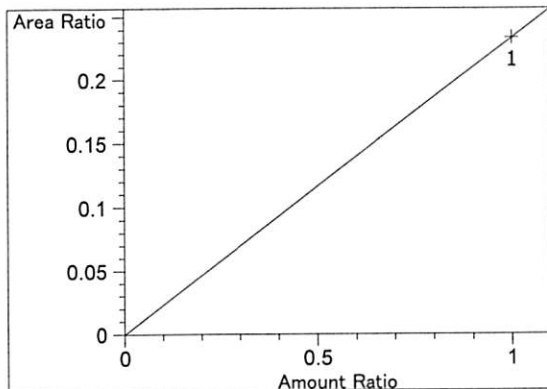

isopropyl alcohol at exp. RT: 4.969
FID2 B, Back Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx + b$
m: 2.33432e-1
b: 0.00000
x: Amount Ratio
y: Area Ratio

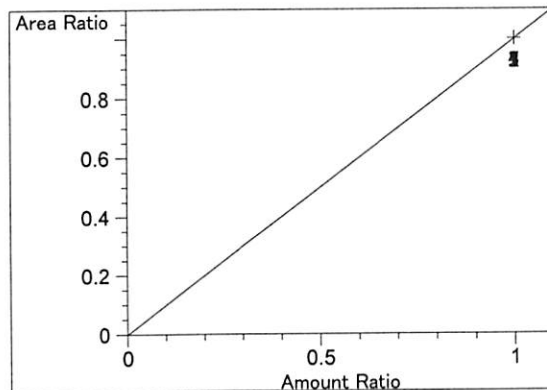


n-propanol at exp. RT: 7.550
FID2 B, Back Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx + b$
m: 1.00000
b: 0.00000
x: Amount Ratio
y: Area Ratio

=====

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.050 FN05211804
 Laboratory : Meridian
 Injection Date : Feb 5, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

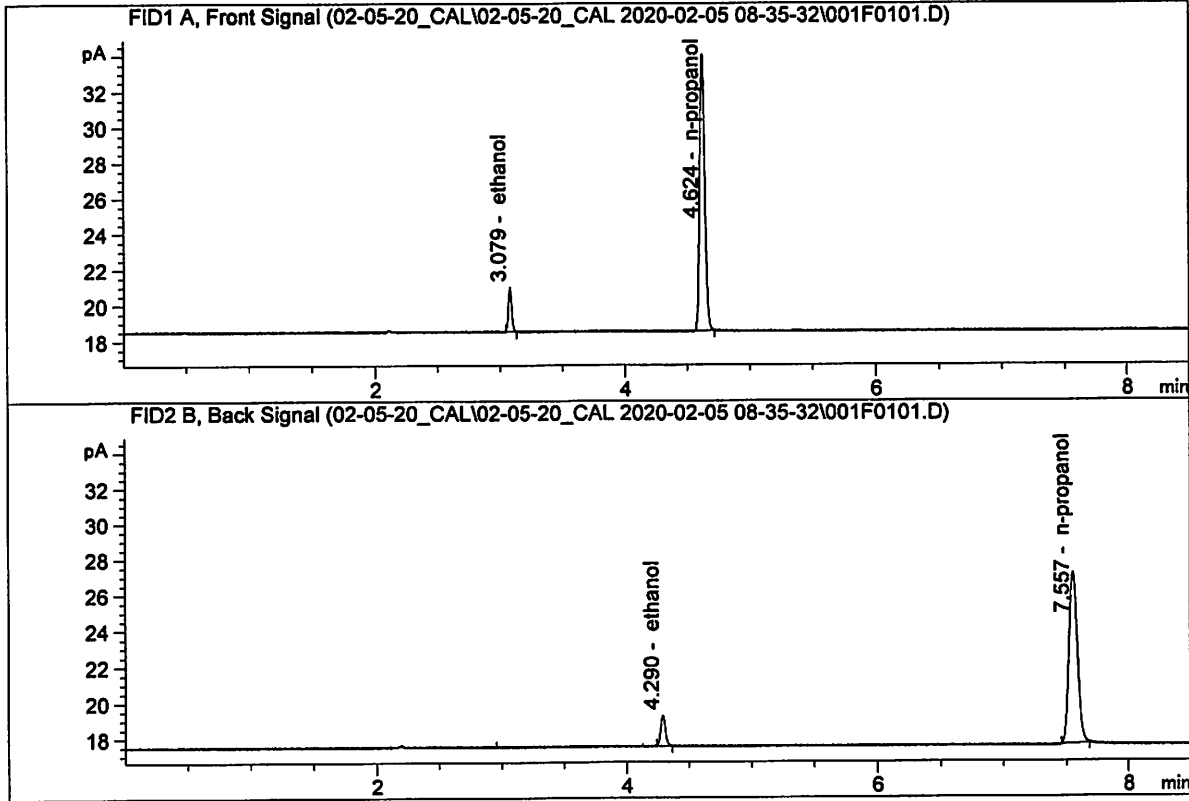


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	4.52242	0.0504	g/100cc
2.	Ethanol	Column 2:	4.62532	0.0518	g/100cc
3.	n-Propanol	Column 1:	44.08209	1.0000	g/100cc
4.	n-Propanol	Column 2:	45.86525	1.0000	g/100cc

W

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.100 FN02271802
 Laboratory : Meridian
 Injection Date : Feb 5, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

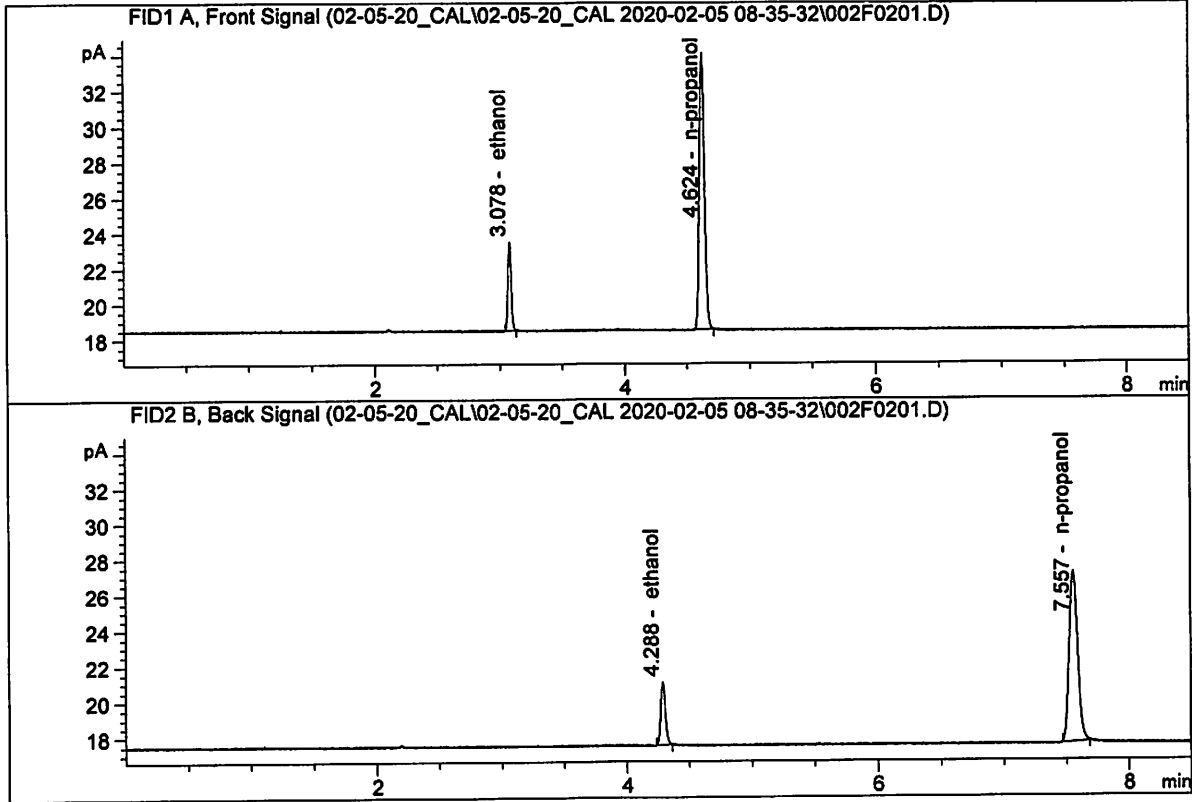


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	9.04952	0.0997	g/100cc
2.	Ethanol	Column 2:	9.39700	0.1005	g/100cc
3.	n-Propanol	Column 1:	44.16013	1.0000	g/100cc
4.	n-Propanol	Column 2:	45.63153	1.0000	g/100cc

W

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.200 FN06231704
 Laboratory : Meridian
 Injection Date : Feb 5, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

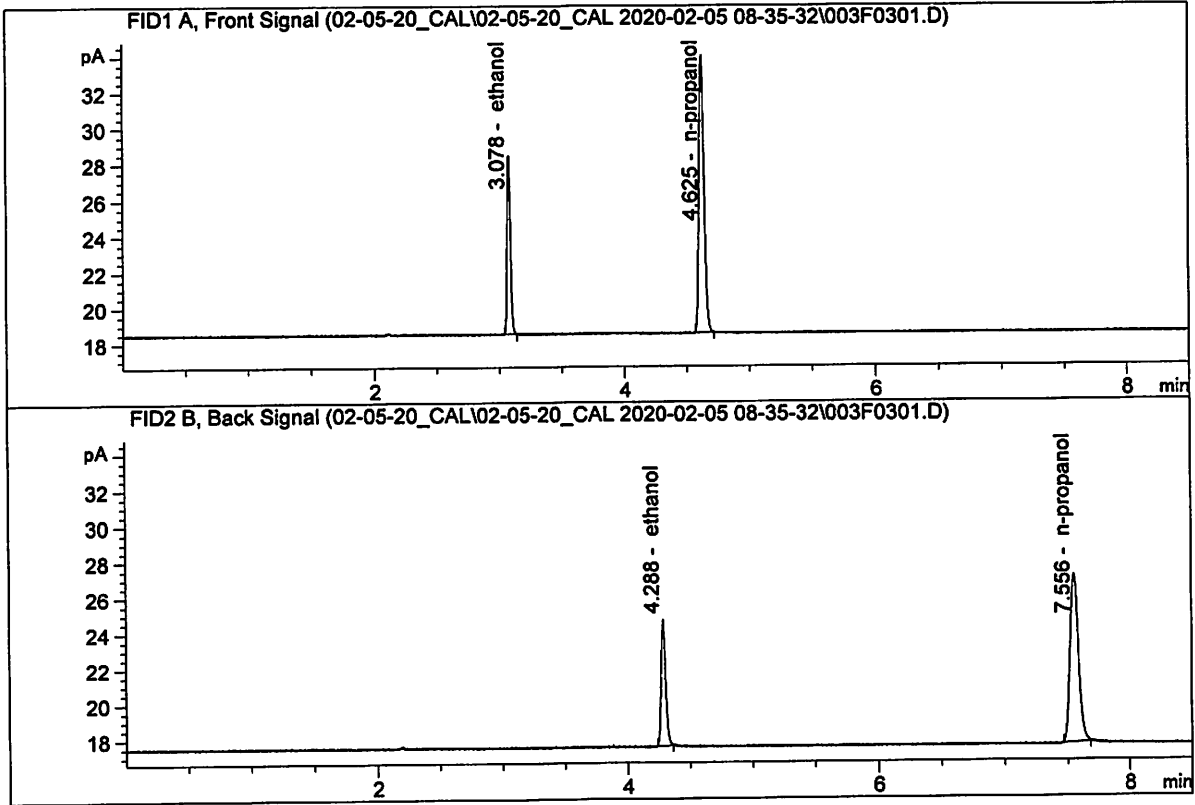


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	18.19493	0.2001	g/100cc
2.	Ethanol	Column 2:	18.84535	0.1980	g/100cc
3.	n-Propanol	Column 1:	44.01959	1.0000	g/100cc
4.	n-Propanol	Column 2:	45.28697	1.0000	g/100cc

W

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.300 FN07311804
 Laboratory : Meridian
 Injection Date : Feb 5, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

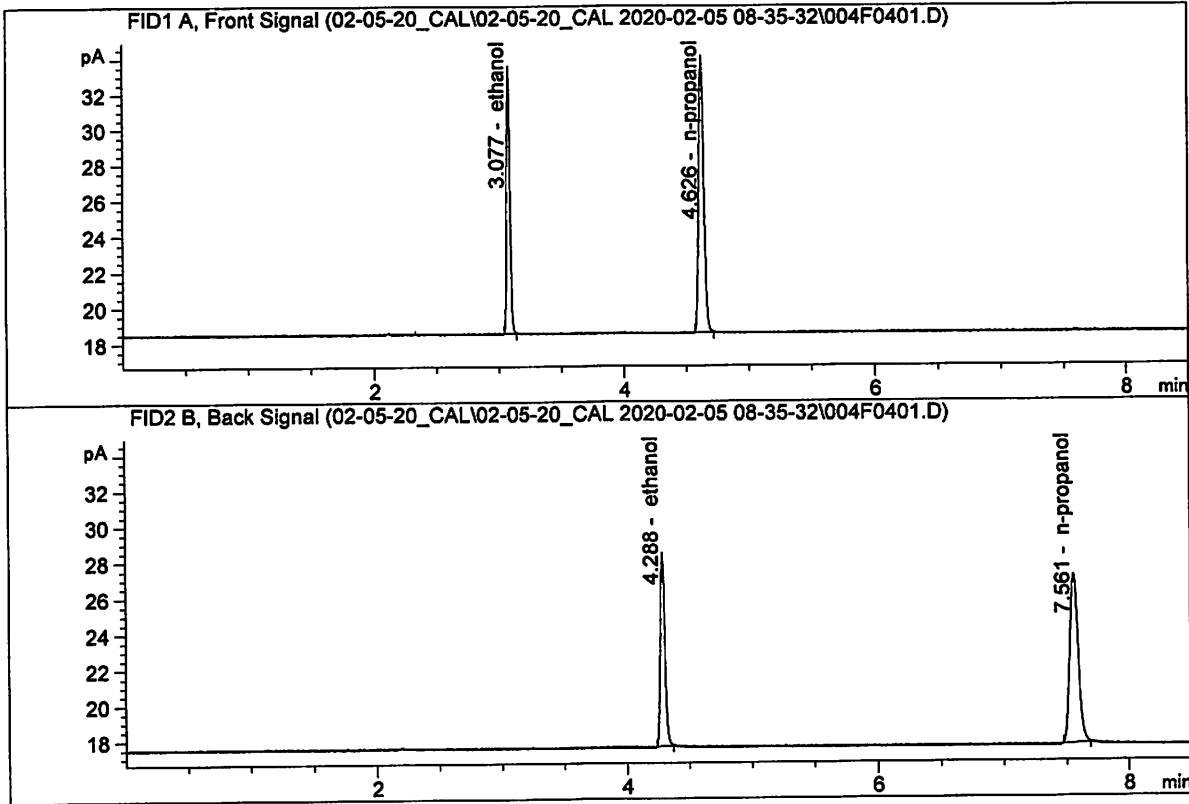


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	27.40895	0.2994	g/100cc
2.	Ethanol	Column 2:	28.70562	0.2980	g/100cc
3.	n-Propanol	Column 1:	44.24614	1.0000	g/100cc
4.	n-Propanol	Column 2:	45.42099	1.0000	g/100cc

W

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.500 FN08031602
 Laboratory : Meridian
 Injection Date : Feb 5, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

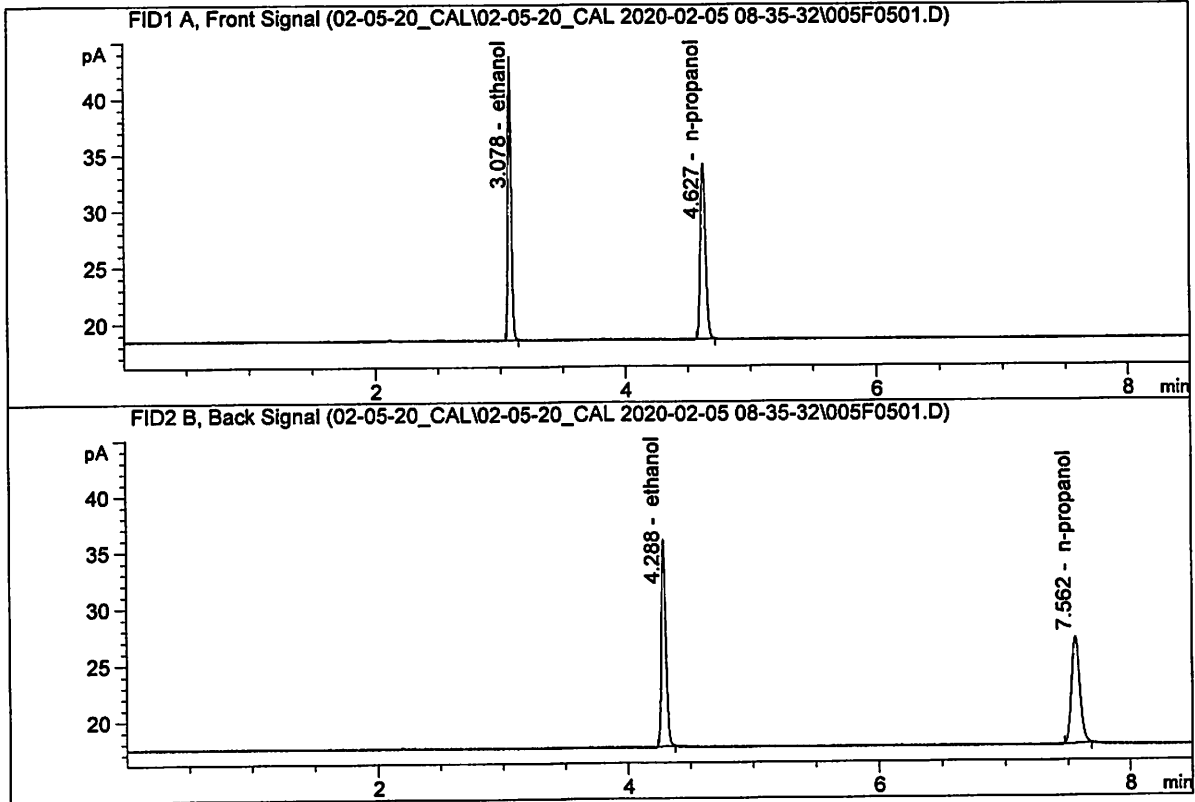


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	45.87756	0.5003	g/100cc
2.	Ethanol	Column 2:	48.52429	0.5017	g/100cc
3.	n-Propanol	Column 1:	44.25955	1.0000	g/100cc
4.	n-Propanol	Column 2:	45.29530	1.0000	g/100cc

W

ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STANDARD BLANK
 Laboratory : Meridian
 Injection Date : Feb 5, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

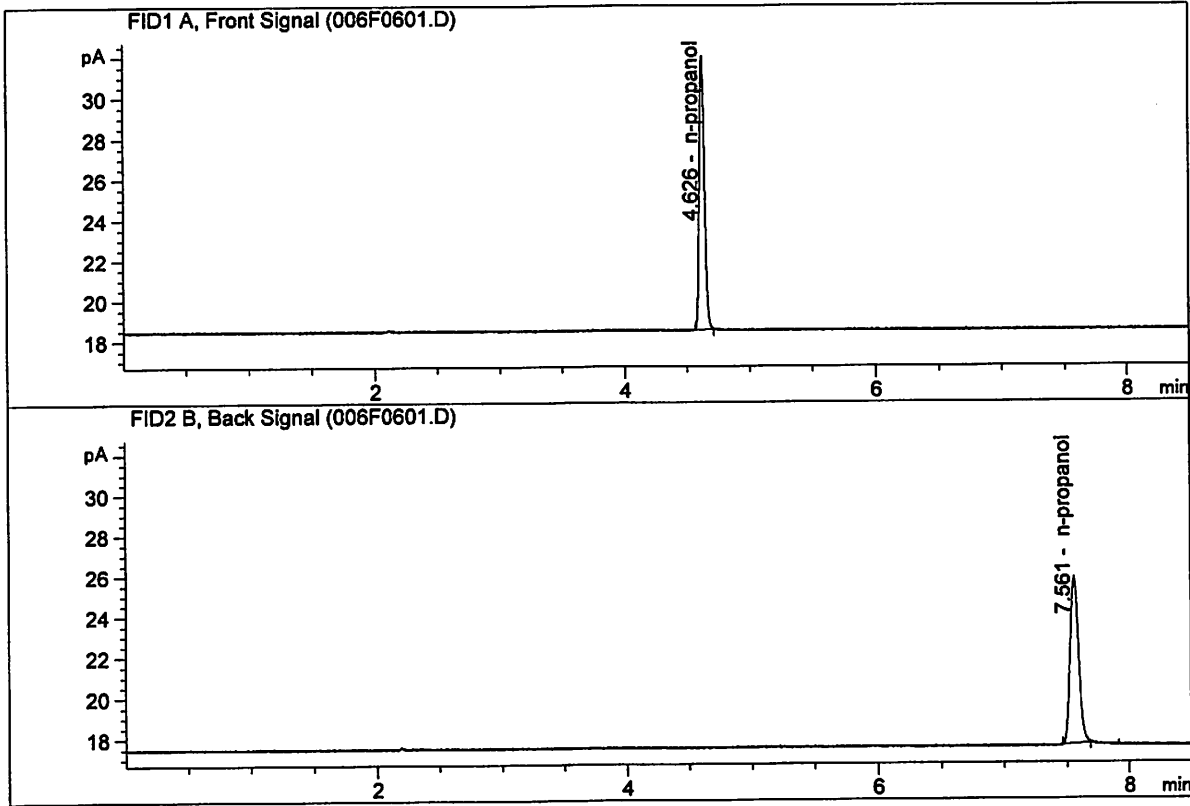

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	38.32483	1.0000	g/100cc
4.	n-Propanol	Column 2:	39.03453	1.0000	g/100cc

W

S a m p l e S u m m a r y


Sequence table: C:\Chem32\1\Data\02-05-20_CAL\02-05-20_CAL 2020-02-05 08-35-32\02-05-20_CAL.S
 Data directory path: C:\Chem32\1\Data\02-05-20_CAL\02-05-20_CAL 2020-02-05 08-35-32\
 Logbook: C:\Chem32\1\Data\02-05-20_CAL\02-05-20_CAL 2020-02-05 08-35-32\02-05-20_CAL.LOG
 Sequence start: 2/5/2020 8:50:11 AM
 Sequence Operator: SYSTEM
 Operator: SYSTEM

Method file name: C:\Chem32\1\Data\02-05-20_CAL\02-05-20_CAL 2020-02-05 08-35-32\ALCOHOL.M

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #	Cmp
1	1	1	0.050 FN05211804	-	1.0000	001F0101.D	*	4
2	2	1	0.100 FN02271802	-	1.0000	002F0201.D	*	4
3	3	1	0.200 FN06231704	-	1.0000	003F0301.D	*	4
4	4	1	0.300 FN07311804	-	1.0000	004F0401.D	*	4
5	5	1	0.500 FN08031602	-	1.0000	005F0501.D	*	4
6	6	1	INTERNAL STANDAR	-	1.0000	006F0601.D		2

ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STD BLK 1
 Laboratory : Meridian
 Injection Date : Feb 5, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

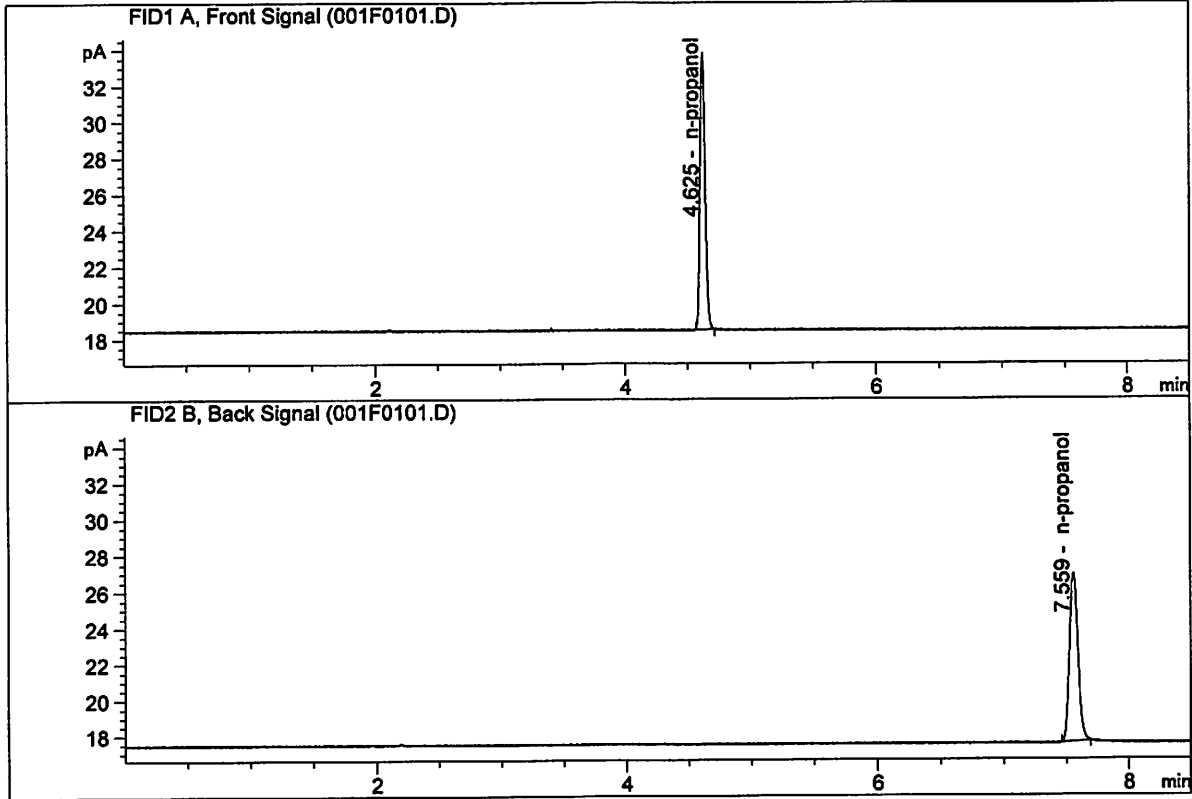


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	43.47083	1.0000	g/100cc
4.	n-Propanol	Column 2:	44.93486	1.0000	g/100cc

W

ISP Forensic Services Blood Alcohol Report

Sample Name : MIX VOL FN06041502
 Laboratory : Meridian
 Injection Date : Feb 5, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

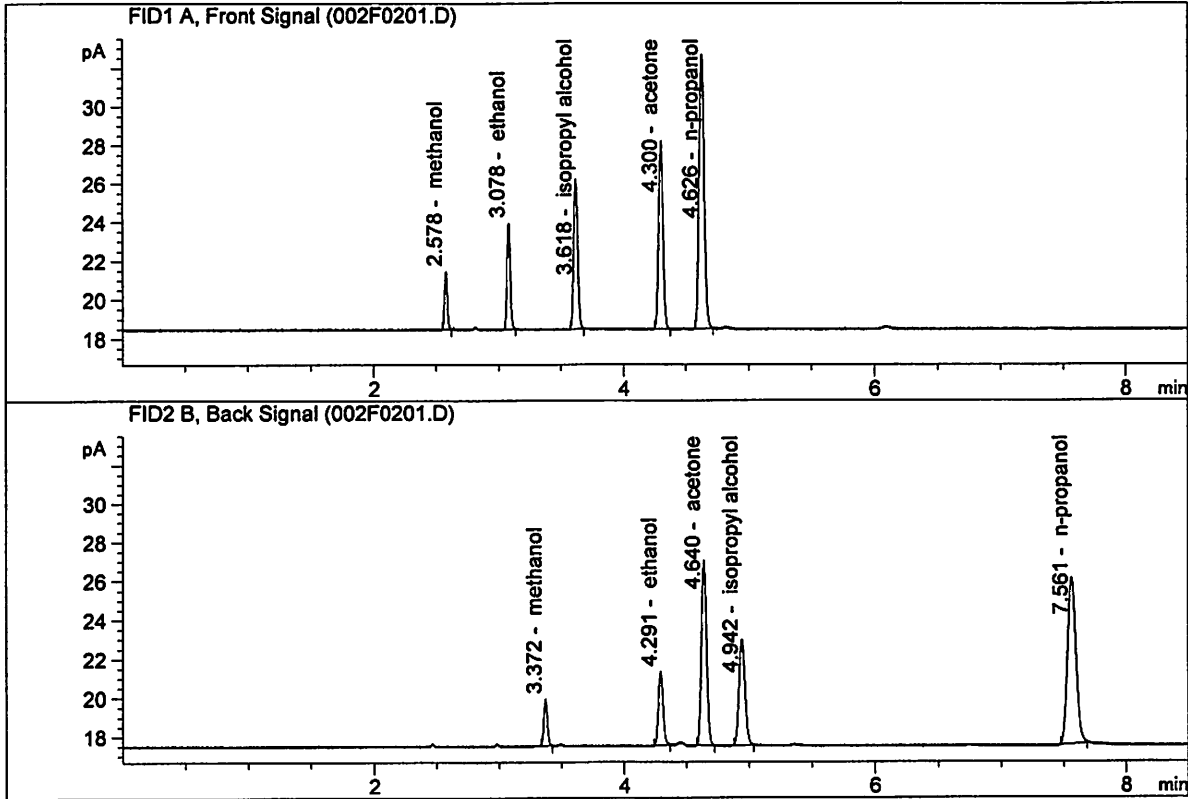

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	9.71600	0.1183	g/100cc
2.	Ethanol	Column 2:	10.00644	0.1190	g/100cc
3.	n-Propanol	Column 1:	39.91807	1.0000	g/100cc
4.	n-Propanol	Column 2:	40.69627	1.0000	g/100cc

W

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC1-1

Analysis Date(s): 05 Feb 2020

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Sample A-B Difference	Over-all Mean
Sample Results	0.0785	0.0795	0.0010	0.0790	0.0001	0.0789
(g/100cc)	0.0790	0.0788	0.0002	0.0789		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument information is stored centrally.

Refer to Instrument Method: Alcohol.m

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.078	0.074	0.082	0.004

	Reported Result	
	0.078	

Calibration and control data are stored centrally.

Revision: 2


Issue Date: 12/23/2019

Issuing Authority: Quality Manager



ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-1-A
 Laboratory : Meridian
 Injection Date : Feb 5, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

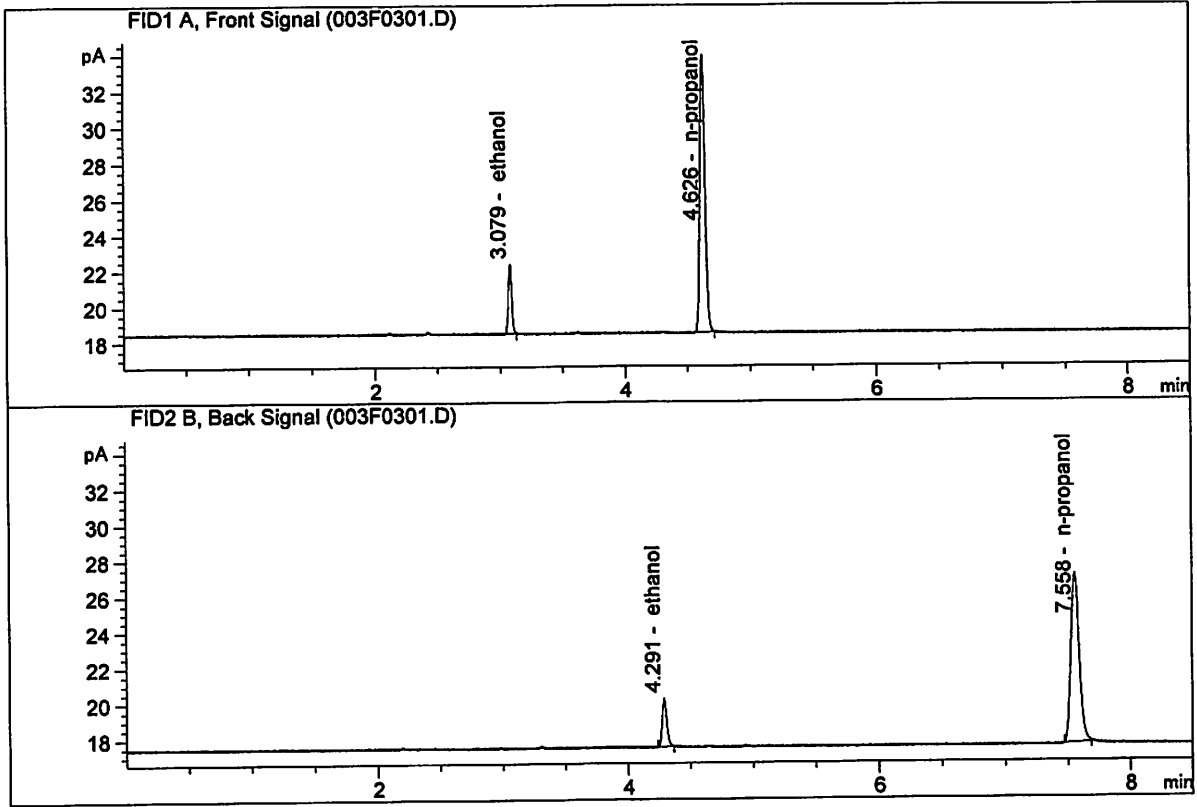


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.06616	0.0785	g/100cc
2.	Ethanol	Column 2:	7.22429	0.0795	g/100cc
3.	n-Propanol	Column 1:	43.92139	1.0000	g/100cc
4.	n-Propanol	Column 2:	44.98053	1.0000	g/100cc

W

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-1-B
 Laboratory : Meridian
 Injection Date : Feb 5, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

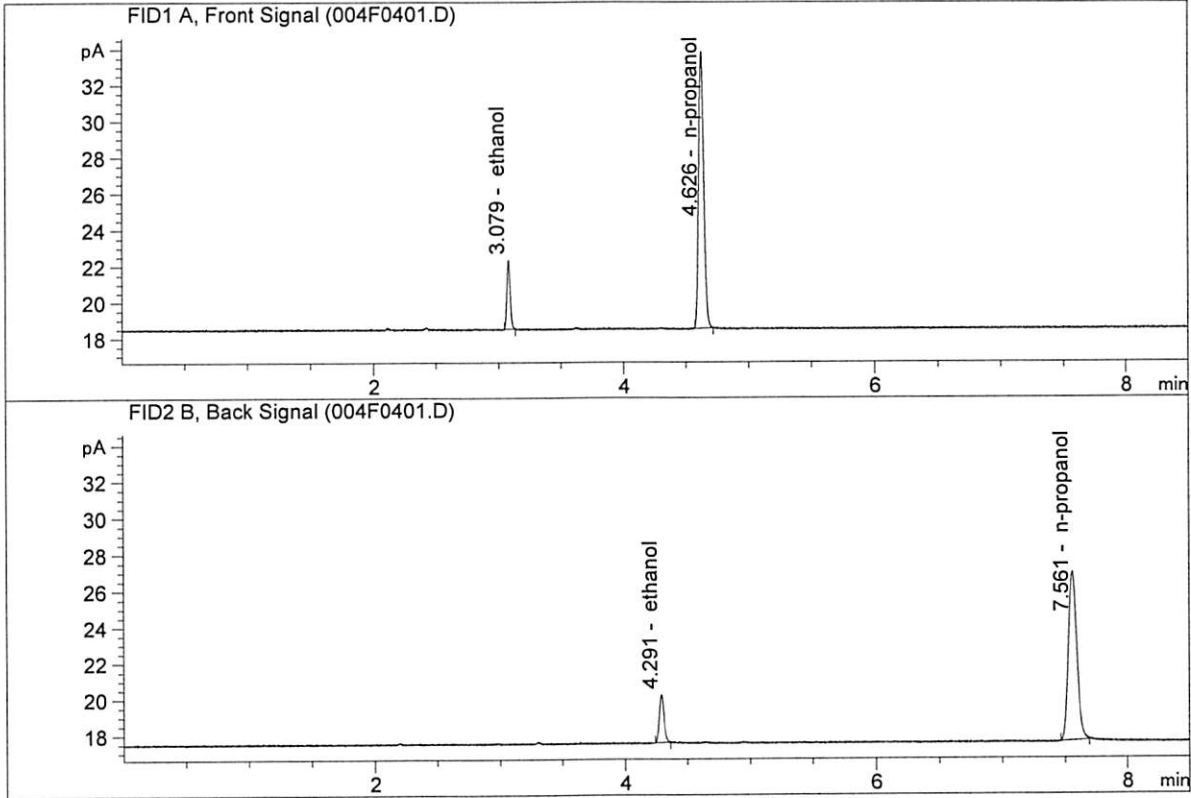

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.04885	0.0790	g/100cc
2.	Ethanol	Column 2:	7.12487	0.0788	g/100cc
3.	n-Propanol	Column 1:	43.55167	1.0000	g/100cc
4.	n-Propanol	Column 2:	44.78526	1.0000	g/100cc

W

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: 0.08 FN04171701

Analysis Date(s): 05 Feb 2020

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Sample A-B Difference	Over-all Mean
Sample Results	0.0801	0.0806	0.0005	0.0803	0.0006	0.0806
(g/100cc)	0.0806	0.0813	0.0007	0.0809		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument information is stored centrally.

Refer to Instrument Method: Alcohol.m

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.080	0.076	0.084	0.004

	Reported Result
	0.080

Calibration and control data are stored centrally.



Revision: 2

Issue Date: 12/23/2019

Issuing Authority: Quality Manager

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.08 FN04171701-A
 Laboratory : Meridian
 Injection Date : Feb 5, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

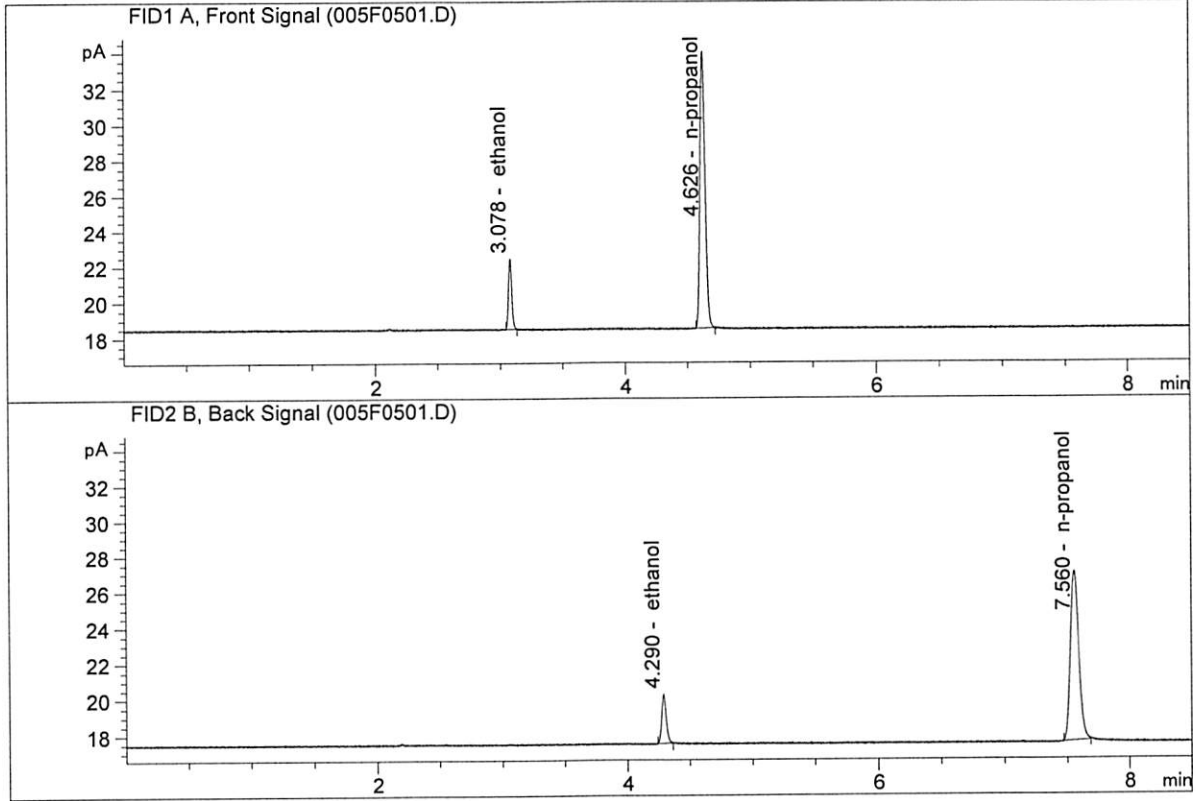


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.23808	0.0801	g/100cc
2.	Ethanol	Column 2:	7.34702	0.0806	g/100cc
3.	n-Propanol	Column 1:	44.09294	1.0000	g/100cc
4.	n-Propanol	Column 2:	45.08530	1.0000	g/100cc

[Handwritten signature]

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.08 FN04171701-B
 Laboratory : Meridian
 Injection Date : Feb 5, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

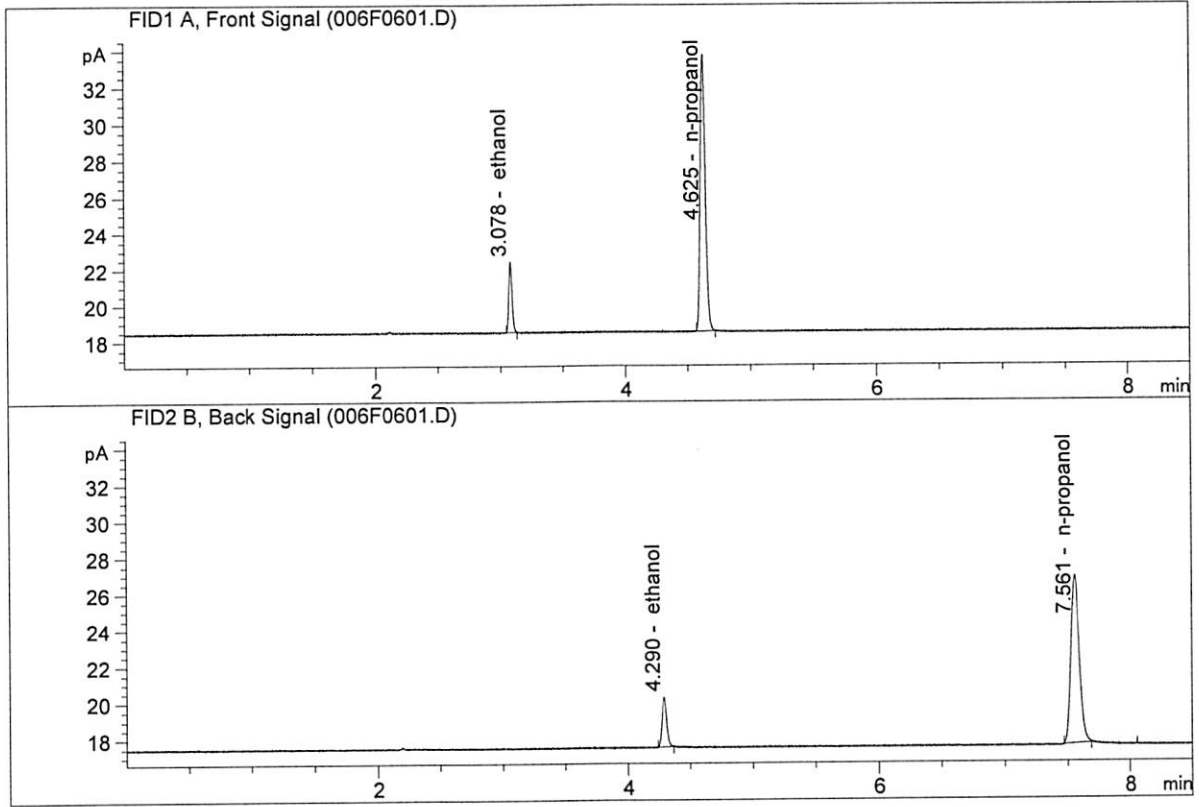

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.13803	0.0806	g/100cc
2.	Ethanol	Column 2:	7.27581	0.0813	g/100cc
3.	n-Propanol	Column 1:	43.21263	1.0000	g/100cc
4.	n-Propanol	Column 2:	44.20213	1.0000	g/100cc

W

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC2-1

Analysis Date(s): 05 Feb 2020

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Sample A-B Difference	Over-all Mean
Sample Results	0.1940	0.1937	0.0003	0.1938	0.0031	0.1954
(g/100cc)	0.1970	0.1969	0.0001	0.1969		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument information is stored centrally.

Refer to Instrument Method: Alcohol.m

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.195	0.185	0.205	0.010


	Reported Result
	0.195

Calibration and control data are stored centrally.

W

ISP Forensic Services Blood Alcohol Report

Sample Name : QC2-1-A
 Laboratory : Meridian
 Injection Date : Feb 5, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

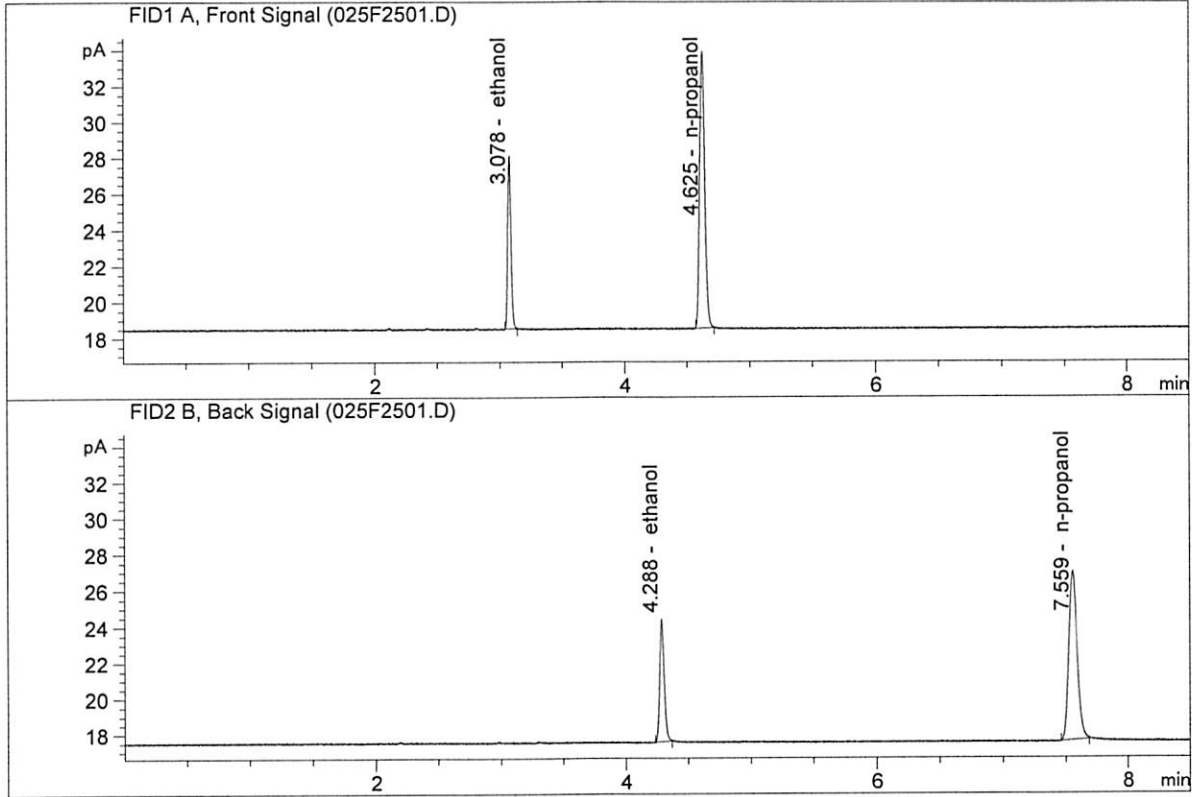


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	17.52965	0.1940	g/100cc
2.	Ethanol	Column 2:	18.22322	0.1937	g/100cc
3.	n-Propanol	Column 1:	43.75341	1.0000	g/100cc
4.	n-Propanol	Column 2:	44.79082	1.0000	g/100cc

W

ISP Forensic Services Blood Alcohol Report

Sample Name : QC2-1-B
 Laboratory : Meridian
 Injection Date : Feb 5, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

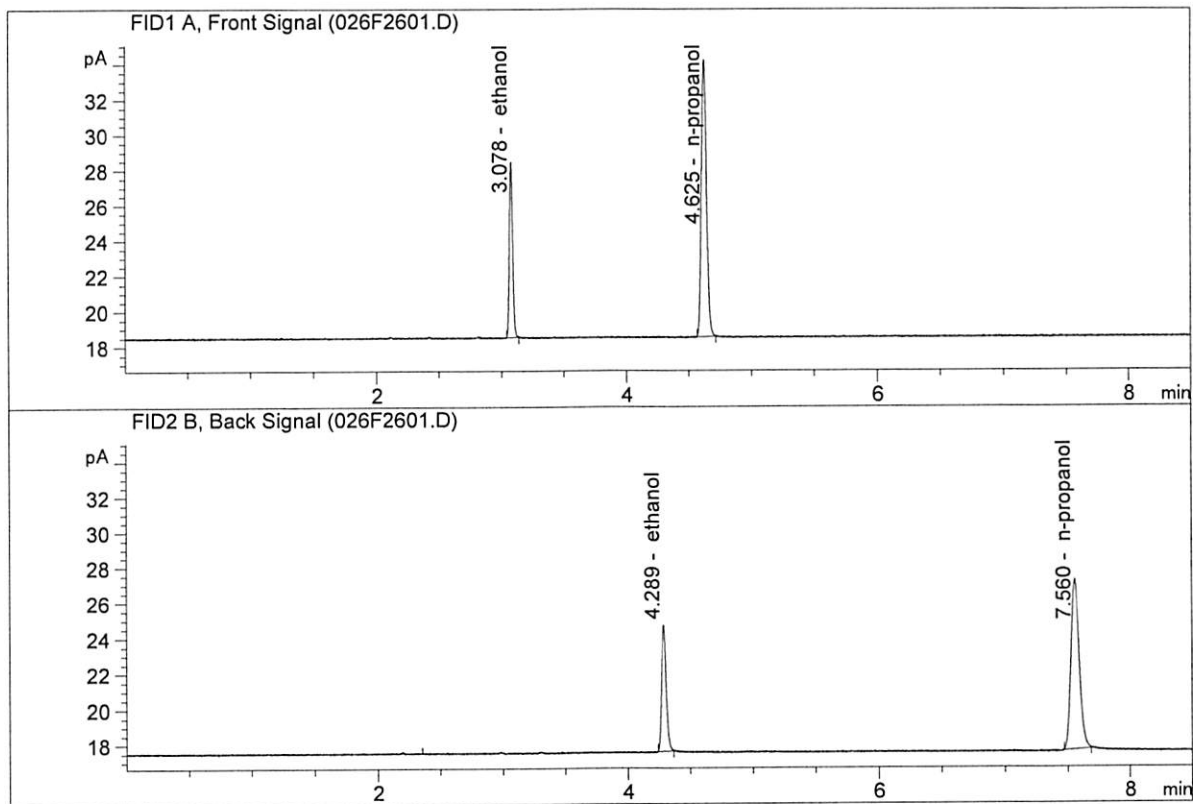

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	18.21442	0.1970	g/100cc
2.	Ethanol	Column 2:	18.91179	0.1969	g/100cc
3.	n-Propanol	Column 1:	44.75841	1.0000	g/100cc
4.	n-Propanol	Column 2:	45.70159	1.0000	g/100cc

W

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC1-2

Analysis Date(s): 05 Feb 2020

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Sample A-B Difference	Over-all Mean
Sample Results	0.0803	0.0813	0.0010	0.0808	0.0003	0.0806
(g/100cc)	0.0801	0.0810	0.0009	0.0805		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument information is stored centrally.

Refer to Instrument Method: Alcohol.m

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.080	0.076	0.084	0.004

	Reported Result	
	0.080	

Calibration and control data are stored centrally.


Revision: 2

Issue Date: 12/23/2019

Issuing Authority: Quality Manager

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-2-A
 Laboratory : Meridian
 Injection Date : Feb 5, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

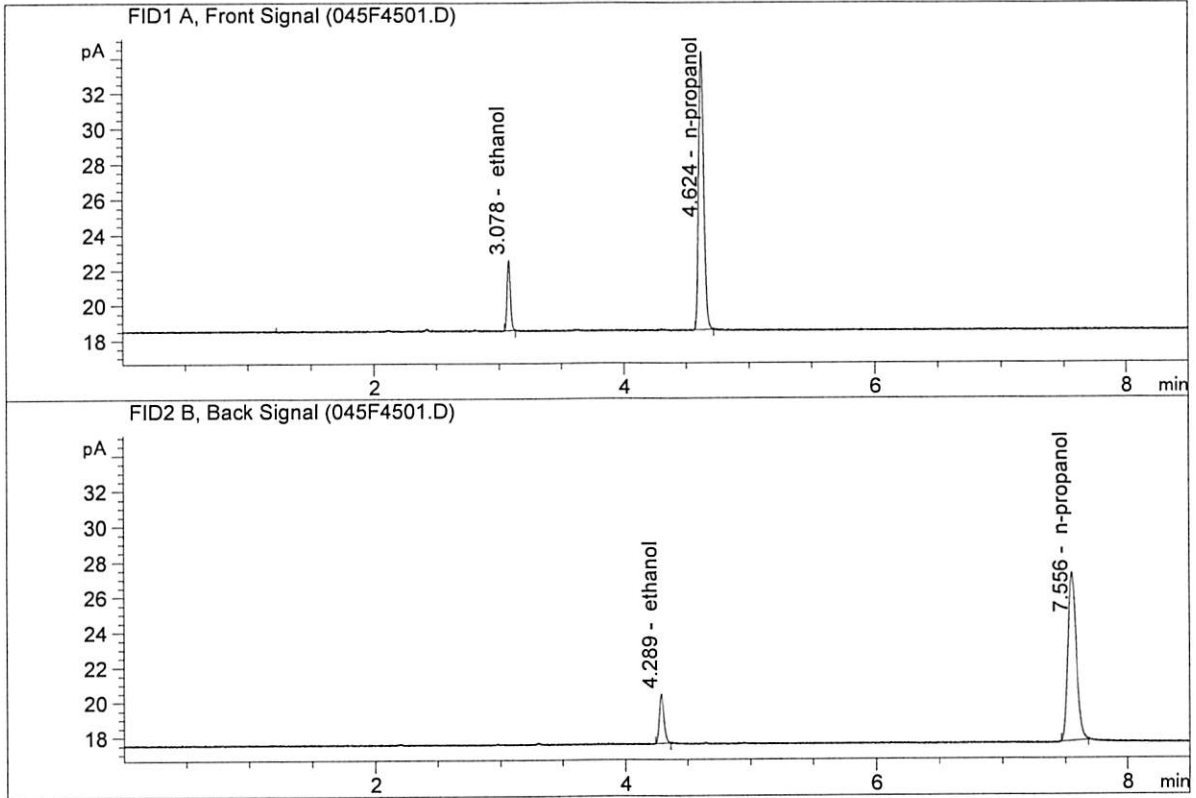


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.36928	0.0803	g/100cc
2.	Ethanol	Column 2:	7.53960	0.0813	g/100cc
3.	n-Propanol	Column 1:	44.77190	1.0000	g/100cc
4.	n-Propanol	Column 2:	45.80434	1.0000	g/100cc

W

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-2-B
 Laboratory : Meridian
 Injection Date : Feb 5, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

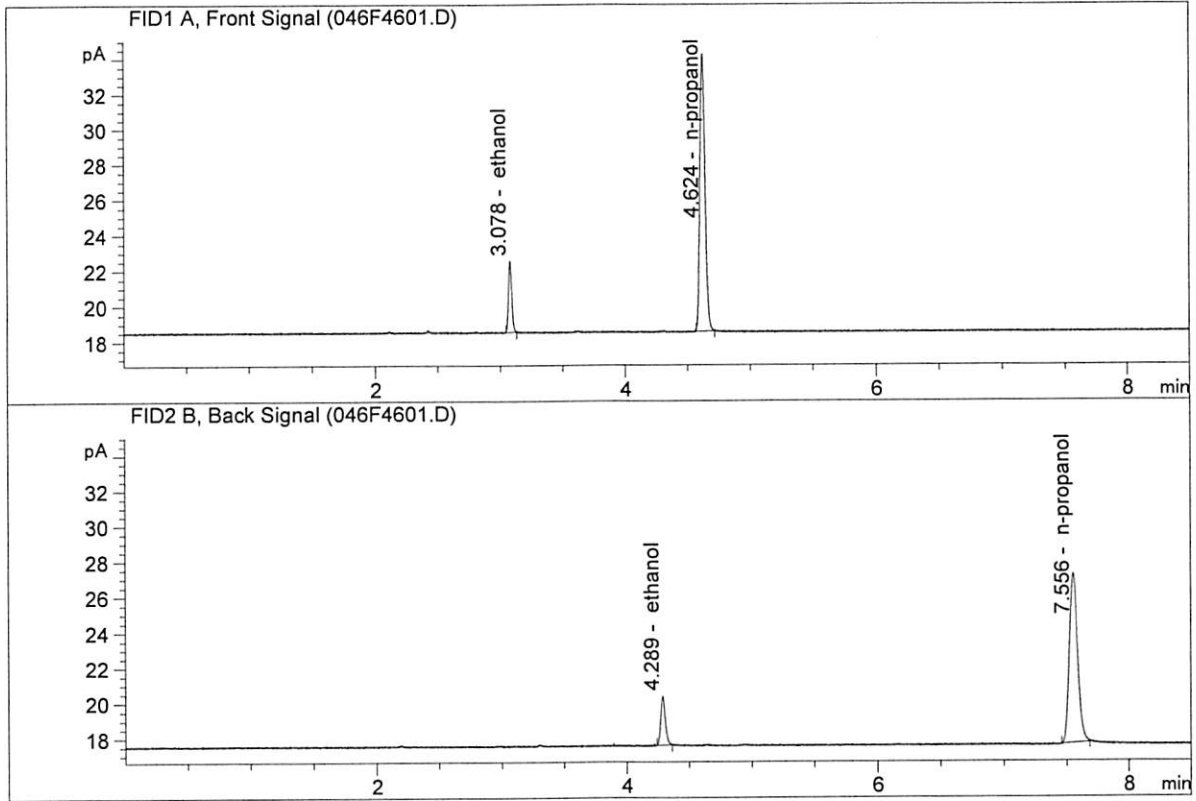


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.31565	0.0801	g/100cc
2.	Ethanol	Column 2:	7.46851	0.0810	g/100cc
3.	n-Propanol	Column 1:	44.53455	1.0000	g/100cc
4.	n-Propanol	Column 2:	45.54882	1.0000	g/100cc

K

ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STD BLK
 Laboratory : Meridian
 Injection Date : Feb 5, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

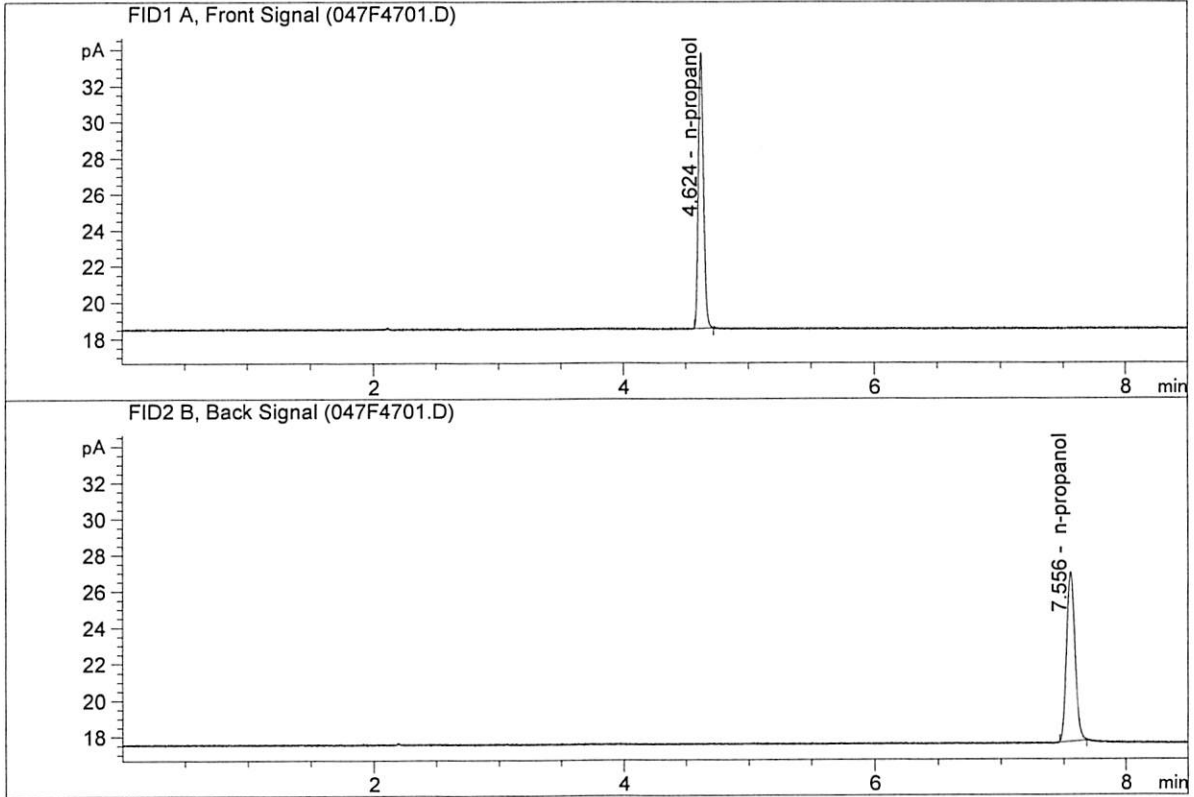

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	43.51861	1.0000	g/100cc
4.	n-Propanol	Column 2:	44.50066	1.0000	g/100cc

W

S a m p l e S u m m a r y

Sequence table: C:\Chem32\1\Data\02-05-20_SAMPLES\02-05-20_SAMPLES 2020-02-05 10-15-27\02-05-20_SAMPLES.S
 Data directory path: C:\Chem32\1\Data\02-05-20_SAMPLES\02-05-20_SAMPLES 2020-02-05 10-15-27\
 Logbook: C:\Chem32\1\Data\02-05-20_SAMPLES\02-05-20_SAMPLES 2020-02-05 10-15-27\02-05-20_SAMPLES.LOG
 Sequence start: 2/5/2020 10:30:12 AM
 Sequence Operator: SYSTEM
 Operator: SYSTEM
 Method file name: C:\Chem32\1\Data\02-05-20_SAMPLES\02-05-20_SAMPLES 2020-02-05 10-15-27\ALCOHOL.M

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #	# Cmp
1	1	1	INTERNAL STD BLK	-	1.0000	001F0101.D		2
2	2	1	MIX VOL FN060415	-	1.0000	002F0201.D		10
3	3	1	QC1-1-A	-	1.0000	003F0301.D		4
4	4	1	QC1-1-B	-	1.0000	004F0401.D		4
5	5	1	0.08 FN04171701-	-	1.0000	005F0501.D		4
6	6	1	0.08 FN04171701-	-	1.0000	006F0601.D		4
7	7	1	M2020-0306-2-A	-	1.0000	007F0701.D		2
8	8	1	M2020-0306-2-B	-	1.0000	008F0801.D		2
9	9	1	M2020-0322-1-A	-	1.0000	009F0901.D		4
10	10	1	M2020-0322-1-B	-	1.0000	010F1001.D		4
11	11	1	M2020-0323-1-A	-	1.0000	011F1101.D		4
12	12	1	M2020-0323-1-B	-	1.0000	012F1201.D		4
13	13	1	M2020-0343-1-A	-	1.0000	013F1301.D		4
14	14	1	M2020-0343-1-B	-	1.0000	014F1401.D		4
15	15	1	M2020-0344-1-A	-	1.0000	015F1501.D		4
16	16	1	M2020-0344-1-B	-	1.0000	016F1601.D		4
17	17	1	M2020-0358-2-A	-	1.0000	017F1701.D		2
18	18	1	M2020-0358-2-B	-	1.0000	018F1801.D		2
19	19	1	M2020-0359-1-A	-	1.0000	019F1901.D		4
20	20	1	M2020-0359-1-B	-	1.0000	020F2001.D		4
21	21	1	M2020-0362-1-A	-	1.0000	021F2101.D		4
22	22	1	M2020-0362-1-B	-	1.0000	022F2201.D		4
23	23	1	M2020-0377-1-A	-	1.0000	023F2301.D		4
24	24	1	M2020-0377-1-B	-	1.0000	024F2401.D		4
25	25	1	QC2-1-A	-	1.0000	025F2501.D		4
26	26	1	QC2-1-B	-	1.0000	026F2601.D		4
27	27	1	M2020-0415-1-A	-	1.0000	027F2701.D		4
28	28	1	M2020-0415-1-B	-	1.0000	028F2801.D		4
29	29	1	M2020-0416-1-A	-	1.0000	029F2901.D		4
30	30	1	M2020-0416-1-B	-	1.0000	030F3001.D		4
31	31	1	M2020-0424-2-A	-	1.0000	031F3101.D		4
32	32	1	M2020-0424-2-B	-	1.0000	032F3201.D		4
33	33	1	M2020-0448-1-A	-	1.0000	033F3301.D		2
34	34	1	M2020-0448-1-B	-	1.0000	034F3401.D		2
35	35	1	M2020-0448-2-A	-	1.0000	035F3501.D		2
36	36	1	M2020-0448-2-B	-	1.0000	036F3601.D		2
37	37	1	M2020-0476-1-A	-	1.0000	037F3701.D		4
38	38	1	M2020-0476-1-B	-	1.0000	038F3801.D		4
39	39	1	M2020-0477-1-A	-	1.0000	039F3901.D		4
40	40	1	M2020-0477-1-B	-	1.0000	040F4001.D		4
41	41	1	M2020-0478-1-A	-	1.0000	041F4101.D		4
42	42	1	M2020-0478-1-B	-	1.0000	042F4201.D		4
43	43	1	M2020-0479-1-A	-	1.0000	043F4301.D		4

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #	# Cmp
44	44	1	M2020-0479-1-B	-	1.0000	044F4401.D	4	4
45	45	1	QC1-2-A	-	1.0000	045F4501.D	4	4
46	46	1	QC1-2-B	-	1.0000	046F4601.D	4	4
47	47	1	INTERNAL STD BLK	-	1.0000	047F4701.D	2	2

Method file name: C:\Chem32\1\Data\02-05-20_SAMPLES\02-05-20_SAMPLES 2020-02-05 10-15-27
 \SHUTDOWN.M

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #	# Cmp
48	48	1	EMPTY	-	1.0000	048F4801.D	0	0