
























Worklist: 1701

<u>LAB_CASE</u>	<u>ITEM</u>	<u>TASK_ID</u>	<u>DESCRIPTION</u>	
C2017-0126	1	78400	AM 8 Blood base neutral confin	
C2017-0500	1	80924	AM 8 Blood base neutral confin	
C2017-0502	1	80566	AM 8 Blood base neutral confin	
M2016-5251	1	79582	AM 8 Blood base neutral confin	
M2017-0295	1	78438	AM 8 Blood base neutral confin	
M2017-0764	2	83459	AM 8 Blood base neutral confin	
M2017-0901	1	78046	AM 8 Blood base neutral confin	
M2017-1116	1	79071	AM 8 Blood base neutral confin	
M2017-1119	1	79077	AM 8 Blood base neutral confin	
M2017-1204	1	79655	AM 8 Blood base neutral confin	
M2017-1204	2	80816	AM 8 Blood base neutral confin	
M2017-1311	1	80090	AM 8 Blood base neutral confin	
M2017-1414	1	80717	AM 8 Blood base neutral confin	
P2017-0413	8	79650	AM 8 Blood base neutral confin	
P2017-0465	3	81183	AM 8 Blood base neutral confin	
P2017-0501	1	78442	AM 8 Blood base neutral confin	
P2017-0511	1	78536	AM 8 Blood base neutral confin	
P2017-0607	1	79493	AM 8 Blood base neutral confin	
P2017-0620	1	79604	AM 8 Blood base neutral confin	
P2017-0635	2	82153	AM 8 Blood base neutral confin	
P2017-0636	2	79683	AM 8 Blood base neutral confin	
P2017-0658	1	79952	AM 8 Blood base neutral confin	
P2017-0663	1	80055	AM 8 Blood base neutral confin	

Worklist: 1701

<u>LAB CASE</u>	<u>ITEM</u>	<u>TASK ID</u>	<u>DESCRIPTION</u>	
P2017-0696	1	80176	AM 8 Blood base neutral confir	
P2017-0715	1	80602	AM 8 Blood base neutral confir	
P2017-0735	1	80731	AM 8 Blood base neutral confir	
P2017-0758	1	80963	AM 8 Blood base neutral confir	
P2017-0863	2	81966	AM 8 Blood base neutral confir	
P2017-0864	1	81969	AM 8 Blood base neutral confir	
P2017-0865	1	81972	AM 8 Blood base neutral confir	
P2017-0881	1	82064	AM 8 Blood base neutral confir	
P2017-0898	1	82137	AM 8 Blood base neutral confir	
P2017-0908	1	82245	AM 8 Blood base neutral confir	
P2017-0966	1	83151	AM 8 Blood base neutral confir	

simulate_sequence.log
 Simulate Run Sequence Fri Apr 28 10:58:08 2017

Instrument Name: Major Mass Spec
 Sequence File: D:\MassHunter\GCMS\1\sequence\RMs.sequence.xml
 Comment: MassHunter sequence
 Operator: ISP\datastor
 Data Path: D:\DATA\CDS\2017\042817\
 Method Path: D:\MassHunter\GCMS\1\methods\

Line	Type	Vials	DataFile	Sample Name
Acquisition Method: BNSB120510.M				
1)	Sample	100	Prerun Solvent Blank	Pre-run Solvent Blank
2)	Sample	1	Negative Control-BN	Negative Control -
...	1013			
3)	Sample	2	Spiked Positive Control-BN	Positive Control
4)	Sample	99	prbLK2	Solvent Blank
Acquisition Method: GBT092509-Delta EMV.M				
5)	Sample	100	Prerun Solvent Blankr	Pre-run Solvent Blank
6)	Sample	1	Negative Control-BNr	Negative Control -
...	1013			
7)	Sample	2	Spiked Positive Control-BNr	Positive Control
8)	Sample	99	prbLK2r	Solvent Blank
Acquisition Method: BNSB120510.M				
9)	Sample	100	M2017-0901-1-BNBLK	Lab No.: M2017-0901-1
10)	Sample	3	M2017-0901-1-BN	Lab No.: M2017-0901-1
Acquisition Method: GBT092509-Delta EMV.M				
11)	Sample	3	M2017-0901-1-BNr	Lab No.: M2017-0901-1
Acquisition Method: BNSB120510.M				
12)	Sample	100	M2017-1116-1-BNBLK	Lab No.: M2017-1116-1
13)	Sample	4	M2017-1116-1-BN	Lab No.: M2017-1116-1
Acquisition Method: GBT092509-Delta EMV.M				
14)	Sample	4	M2017-1116-1-BNr	Lab No.: M2017-1116-1
Acquisition Method: BNSB120510.M				
15)	Sample	100	M2017-1119-1-BNBLK	Lab No.: M2017-1119-1
16)	Sample	5	M2017-1119-1-BN	Lab No.: M2017-1119-1
Acquisition Method: GBT092509-Delta EMV.M				
17)	Sample	5	M2017-1119-1-BNr	Lab No.: M2017-1119-1
Acquisition Method: BNSB120510.M				
18)	Sample	100	M2017-1204-1-BNBLK	Lab No.: M2017-1204-1
19)	Sample	6	M2017-1204-1-BN	Lab No.: M2017-1204-1
Acquisition Method: GBT092509-Delta EMV.M				
20)	Sample	6	M2017-1204-1-BNr	Lab No.: M2017-1204-1
Acquisition Method: BNSB120510.M				
21)	Sample	100	M2017-1204-2-BNBLK	Lab No.: M2017-1204-2
22)	Sample	7	M2017-1204-2-BN	Lab No.: M2017-1204-2
Acquisition Method: GBT092509-Delta EMV.M				
23)	Sample	7	M2017-1204-2-BNr	Lab No.: M2017-1204-2
Acquisition Method: BNSB120510.M				
24)	Sample	100	M2017-1311-1-BNBLK	Lab No.: M2017-1311-1
25)	Sample	8	M2017-1311-1-BN	Lab No.: M2017-1311-1
Acquisition Method: GBT092509-Delta EMV.M				
26)	Sample	8	M2017-1311-1-BNr	Lab No.: M2017-1311-1

simulate_sequence.log

Acquisition Method:	BNSB120510.M		
27) Sample	100	M2017-1414-1-BNBLK	Lab No.: M2017-1414-1
28) Sample	9	M2017-1414-1-BN	Lab No.: M2017-1414-1
Acquisition Method:	GBT092509-Delta EMV.M		
29) Sample	9	M2017-1414-1-BNr	Lab No.: M2017-1414-1
Acquisition Method:	BNSB120510.M		
30) Sample	100	P2017-0413-8-BNBLK	Lab No.: P2017-0413-8
31) Sample	10	P2017-0413-8-BN	Lab No.: P2017-0413-8
Acquisition Method:	GBT092509-Delta EMV.M		
32) Sample	10	P2017-0413-8-BNr	Lab No.: P2017-0413-8
Acquisition Method:	BNSB120510.M		
33) Sample	100	P2017-0465-3-BNBLK	Lab No.: P2017-0465-3
34) Sample	11	P2017-0465-3-BN	Lab No.: P2017-0465-3
Acquisition Method:	GBT092509-Delta EMV.M		
35) Sample	11	P2017-0465-3-BNr	Lab No.: P2017-0465-3
Acquisition Method:	BNSB120510.M		
36) Sample	100	P2017-0501-1-BNBLK	Lab No.: P2017-0501-1
37) Sample	12	P2017-0501-1-BN	Lab No.: P2017-0501-1
Acquisition Method:	GBT092509-Delta EMV.M		
38) Sample	12	P2017-0501-1-BNr	Lab No.: P2017-0501-1
Acquisition Method:	BNSB120510.M		
39) Sample	100	P2017-0511-1-BNBLK	Lab No.: P2017-0511-1
40) Sample	13	P2017-0511-1-BN	Lab No.: P2017-0511-1
Acquisition Method:	GBT092509-Delta EMV.M		
41) Sample	13	P2017-0511-1-BNr	Lab No.: P2017-0511-1
Acquisition Method:	BNSB120510.M		
42) Sample	100	P2017-0607-1-BNBLK	Lab No.: P2017-0607-1
43) Sample	14	P2017-0607-1-BN	Lab No.: P2017-0607-1
Acquisition Method:	GBT092509-Delta EMV.M		
44) Sample	14	P2017-0607-1-BNr	Lab No.: P2017-0607-1
Acquisition Method:	BNSB120510.M		
45) Sample	100	P2017-0620-1-BNBLK	Lab No.: P2017-0620-1
46) Sample	15	P2017-0620-1-BN	Lab No.: P2017-0620-1
Acquisition Method:	GBT092509-Delta EMV.M		
47) Sample	15	P2017-0620-1-BNr	Lab No.: P2017-0620-1
Acquisition Method:	BNSB120510.M		
48) Sample	99	P2017-0635-2-BNBLK	Lab No.: P2017-0635-2
49) Sample	16	P2017-0635-2-BN	Lab No.: P2017-0635-2
Acquisition Method:	GBT092509-Delta EMV.M		
50) Sample	16	P2017-0635-2-BNr	Lab No.: P2017-0635-2
Acquisition Method:	BNSB120510.M		
51) Sample	99	P2017-0636-2-BNBLK	Lab No.: P2017-0636-2
52) Sample	17	P2017-0636-2-BN	Lab No.: P2017-0636-2
Acquisition Method:	GBT092509-Delta EMV.M		
53) Sample	17	P2017-0636-2-BNr	Lab No.: P2017-0636-2
Acquisition Method:	BNSB120510.M		
54) Sample	99	P2017-0658-1-BNBLK	Lab No.: P2017-0658-1
55) Sample	18	P2017-0658-1-BN	Lab No.: P2017-0658-1


simulate_sequence.log			
Acquisition Method:	GBT092509-Delta EMV.M		
56) Sample	18	P2017-0658-1-BNr	Lab No.: P2017-0658-1
Acquisition Method:	BNSB120510.M		
57) Sample	99	P2017-0663-1-BNBLK	Lab No.: P2017-0663-1
58) Sample	19	P2017-0663-1-BN	Lab No.: P2017-0663-1
Acquisition Method:	GBT092509-Delta EMV.M		
59) Sample	19	P2017-0663-1-BNr	Lab No.: P2017-0663-1
Acquisition Method:	BNSB120510.M		
60) Sample	99	P2017-0696-1-BNBLK	Lab No.: P2017-0696-1
61) Sample	20	P2017-0696-1-BN	Lab No.: P2017-0696-1
Acquisition Method:	GBT092509-Delta EMV.M		
62) Sample	20	P2017-0696-1-BNr	Lab No.: P2017-0696-1
Acquisition Method:	BNSB120510.M		
63) Sample	99	P2017-0715-1-BNBLK	Lab No.: P2017-0715-1
64) Sample	21	P2017-0715-1-BN	Lab No.: P2017-0715-1
Acquisition Method:	GBT092509-Delta EMV.M		
65) Sample	21	P2017-0715-1-BNr	Lab No.: P2017-0715-1
Acquisition Method:	BNSB120510.M		
66) Sample	99	P2017-0735-1-BNBLK	Lab No.: P2017-0735-1
67) Sample	22	P2017-0735-1-BN	Lab No.: P2017-0735-1
Acquisition Method:	GBT092509-Delta EMV.M		
68) Sample	22	P2017-0735-1-BNr	Lab No.: P2017-0735-1
Acquisition Method:	BNSB120510.M		
69) Sample	99	P2017-0758-1-BNBLK	Lab No.: P2017-0758-1
70) Sample	23	P2017-0758-1-BN	Lab No.: P2017-0758-1
Acquisition Method:	GBT092509-Delta EMV.M		
71) Sample	23	P2017-0758-1-BNr	Lab No.: P2017-0758-1
Acquisition Method:	BNSB120510.M		
72) Sample	99	P2017-0863-2-BNBLK	Lab No.: P2017-0863-2
73) Sample	24	P2017-0863-2-BN	Lab No.: P2017-0863-2
Acquisition Method:	GBT092509-Delta EMV.M		
74) Sample	24	P2017-0863-2-BNr	Lab No.: P2017-0863-2
Acquisition Method:	BNSB120510.M		
75) Sample	99	P2017-0864-1-BNBLK	Lab No.: P2017-0864-1
76) Sample	25	P2017-0864-1-BN	Lab No.: P2017-0864-1
Acquisition Method:	GBT092509-Delta EMV.M		
77) Sample	25	P2017-0864-1-BNr	Lab No.: P2017-0864-1
Acquisition Method:	BNSB120510.M		
78) Sample	99	P2017-0865-1-BNBLK	Lab No.: P2017-0865-1
79) Sample	26	P2017-0865-1-BN	Lab No.: P2017-0865-1
Acquisition Method:	GBT092509-Delta EMV.M		
80) Sample	26	P2017-0865-1-BNr	Lab No.: P2017-0865-1
Acquisition Method:	BNSB120510.M		
81) Sample	99	P2017-0881-1-BNBLK	Lab No.: P2017-0881-1
82) Sample	27	P2017-0881-1-BN	Lab No.: P2017-0881-1
Acquisition Method:	GBT092509-Delta EMV.M		
83) Sample	27	P2017-0881-1-BNr	Lab No.: P2017-0881-1
Acquisition Method:	BNSB120510.M		
84) Sample	99	P2017-0898-1-BNBLK	Lab No.: P2017-0898-1

```

simulate_sequence.log
85) Sample          28          P2017-0898-1-BN          Lab No.: P2017-0898-1
Acquisition Method: GBT092509-Delta EMV.M
86) Sample          28          P2017-0898-1-BNr        Lab No.: P2017-0898-1
Acquisition Method: BNSB120510.M
87) Sample          99          P2017-0908-1-BNBLK     Lab No.: P2017-0908-1
88) Sample          29          P2017-0908-1-BN        Lab No.: P2017-0908-1
Acquisition Method: GBT092509-Delta EMV.M
89) Sample          29          P2017-0908-1-BNr        Lab No.: P2017-0908-1
Acquisition Method: BNSB120510.M
90) Sample          99          P2017-0966-1-BNBLK     Lab No.: P2017-0966-1
91) Sample          30          P2017-0966-1-BN        Lab No.: P2017-0966-1
Acquisition Method: GBT092509-Delta EMV.M
92) Sample          30          P2017-0966-1-BNr        Lab No.: P2017-0966-1
Acquisition Method: BNSB120510.M
93) Sample          99          C2017-0126-1-BNBLK     Lab No.: C2017-0126-1
94) Sample          31          C2017-0126-1-BN        Lab No.: C2017-0126-1
Acquisition Method: GBT092509-Delta EMV.M
95) Sample          31          C2017-0126-1-BNr        Lab No.: C2017-0126-1
Acquisition Method: BNSB120510.M
96) Sample          99          C2017-0500-1-BNBLK     Lab No.: C2017-0500-1
97) Sample          32          C2017-0500-1-BN        Lab No.: C2017-0500-1
Acquisition Method: GBT092509-Delta EMV.M
98) Sample          32          C2017-0500-1-BNr        Lab No.: C2017-0500-1
Acquisition Method: BNSB120510.M
99) Sample          99          C2017-0502-1-BNBLK     Lab No.: C2017-0502-1
100) Sample         33          C2017-0502-1-BN        Lab No.: C2017-0502-1
Acquisition Method: GBT092509-Delta EMV.M
101) Sample         33          C2017-0502-1-BNr        Lab No.: C2017-0502-1
Acquisition Method: BNSB120510.M
102) Sample         99          M2016-5251-1-BNBLK     Lab No.: M2016-5251-1
103) Sample         34          M2016-5251-1-BN        Lab No.: M2016-5251-1
Acquisition Method: GBT092509-Delta EMV.M
104) Sample         34          M2016-5251-1-BNr        Lab No.: M2016-5251-1
Acquisition Method: BNSB120510.M
105) Sample         99          M2017-0295-1-BNBLK     Lab No.: M2017-0295-1
106) Sample         35          M2017-0295-1-BN        Lab No.: M2017-0295-1
Acquisition Method: GBT092509-Delta EMV.M
107) Sample         35          M2017-0295-1-BNr        Lab No.: M2017-0295-1
Acquisition Method: BNSB120510.M
108) Sample         99          M2017-0764-2-BNBLK     Lab No.: M2017-0764-2
109) Sample         36          M2017-0764-2-BN        Lab No.: M2017-0764-2
Acquisition Method: GBT092509-Delta EMV.M
110) Sample         36          M2017-0764-2-BNr        Lab No.: M2017-0764-2
Acquisition Method: BNSB120510.M
111) Sample         99          POSTBLK                 BLK
Acquisition Method: GBT092509-Delta EMV.M
112) Sample         99          AFTER                   BLK
megabytes Needed: 1514 Space on drive D: 188620
Sequence Verification Done!



```

File :I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2017\042817
... \Negative Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 28 Apr 2017 11:25 using AcqMethod BNSB120510.M
Sample Name: Negative Control - Utak Lot B1013
Misc Info : UTAK B1013


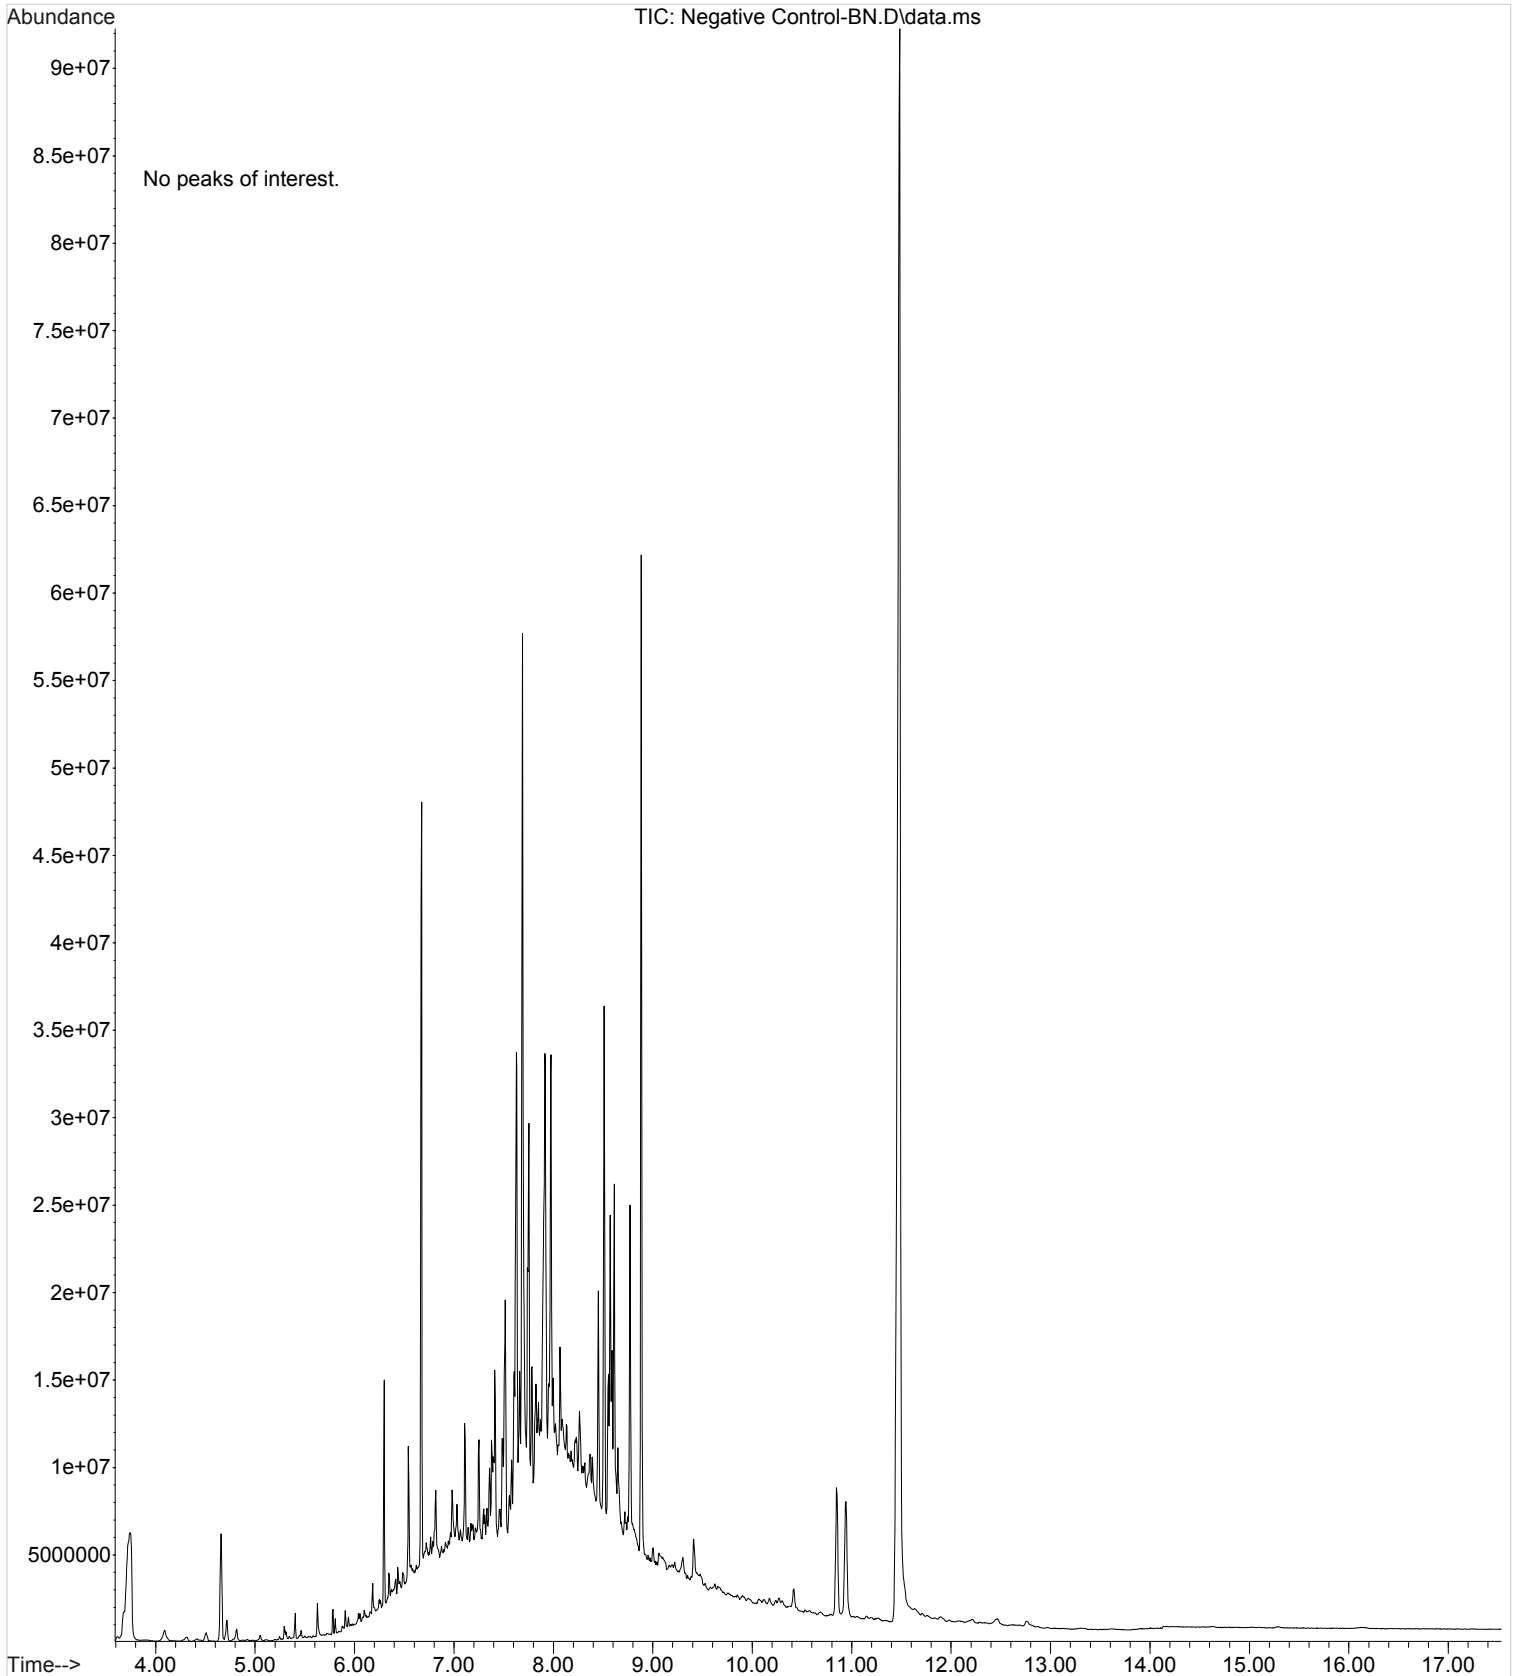


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2017\042817
... \Negative Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 28 Apr 2017 11:25 using AcqMethod BNSB120510.M
Sample Name: Negative Control - Utak Lot B1013
Misc Info : UTAK B1013


9

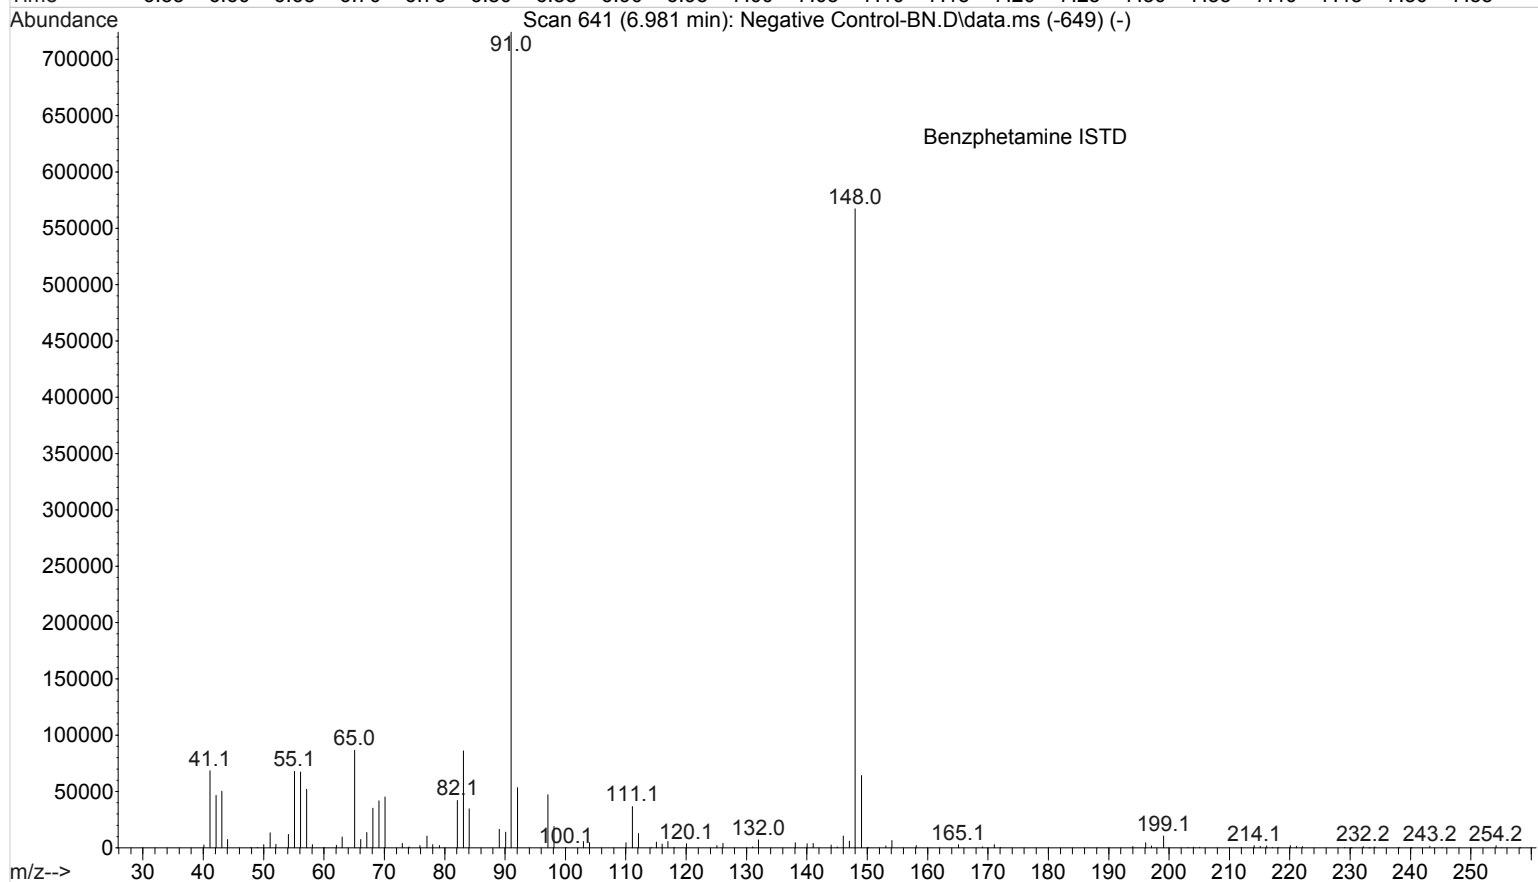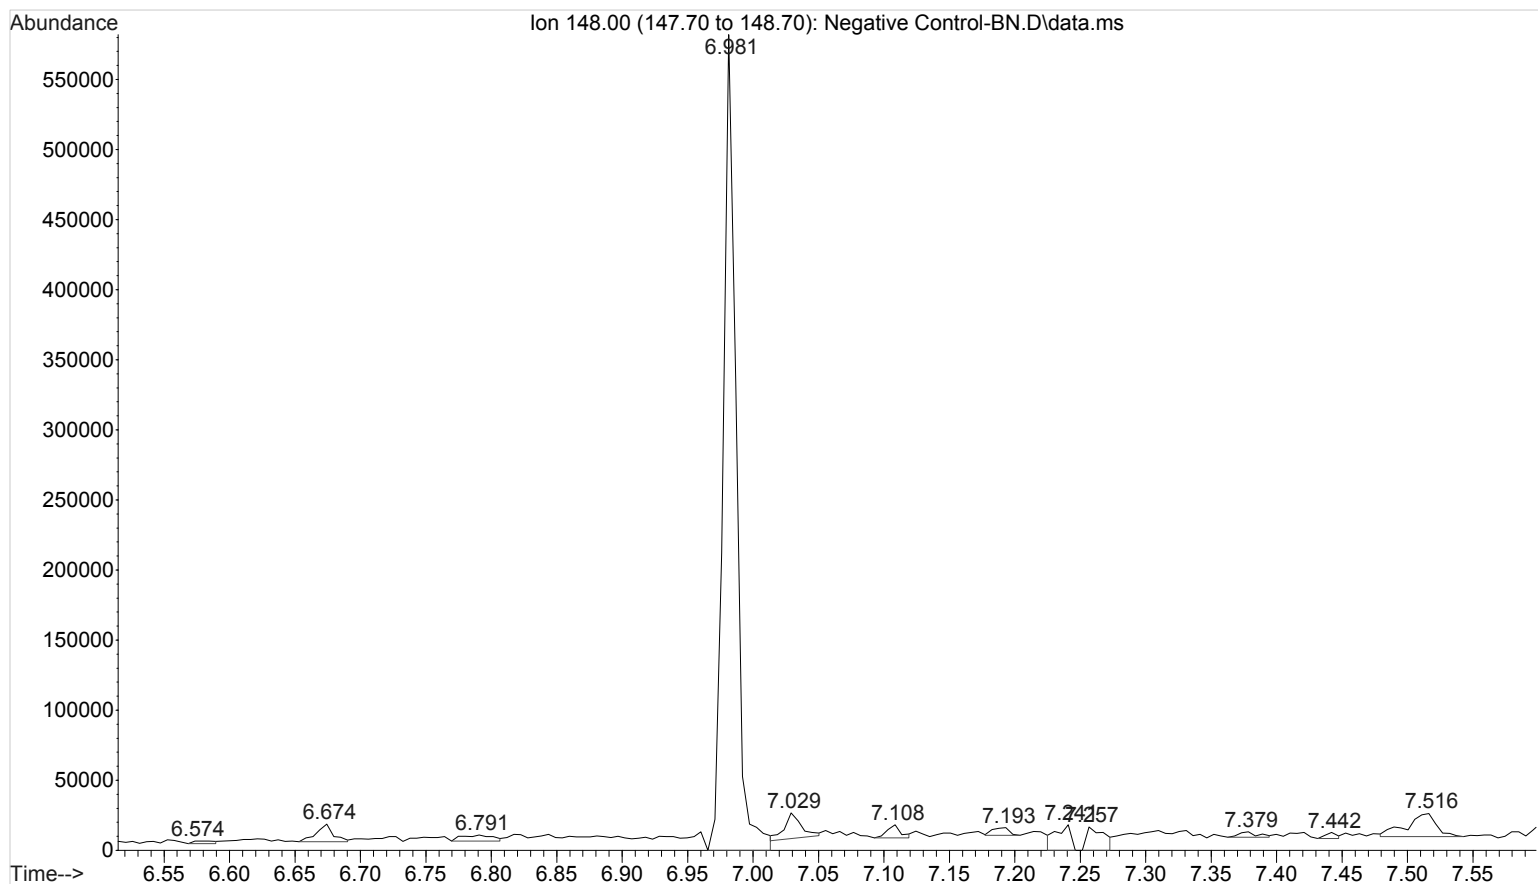



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2017\042817
... \Negative Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 28 Apr 2017 11:25 using AcqMethod BNSB120510.M
Sample Name: Negative Control - Utak Lot B1013
Misc Info : UTAK B1013

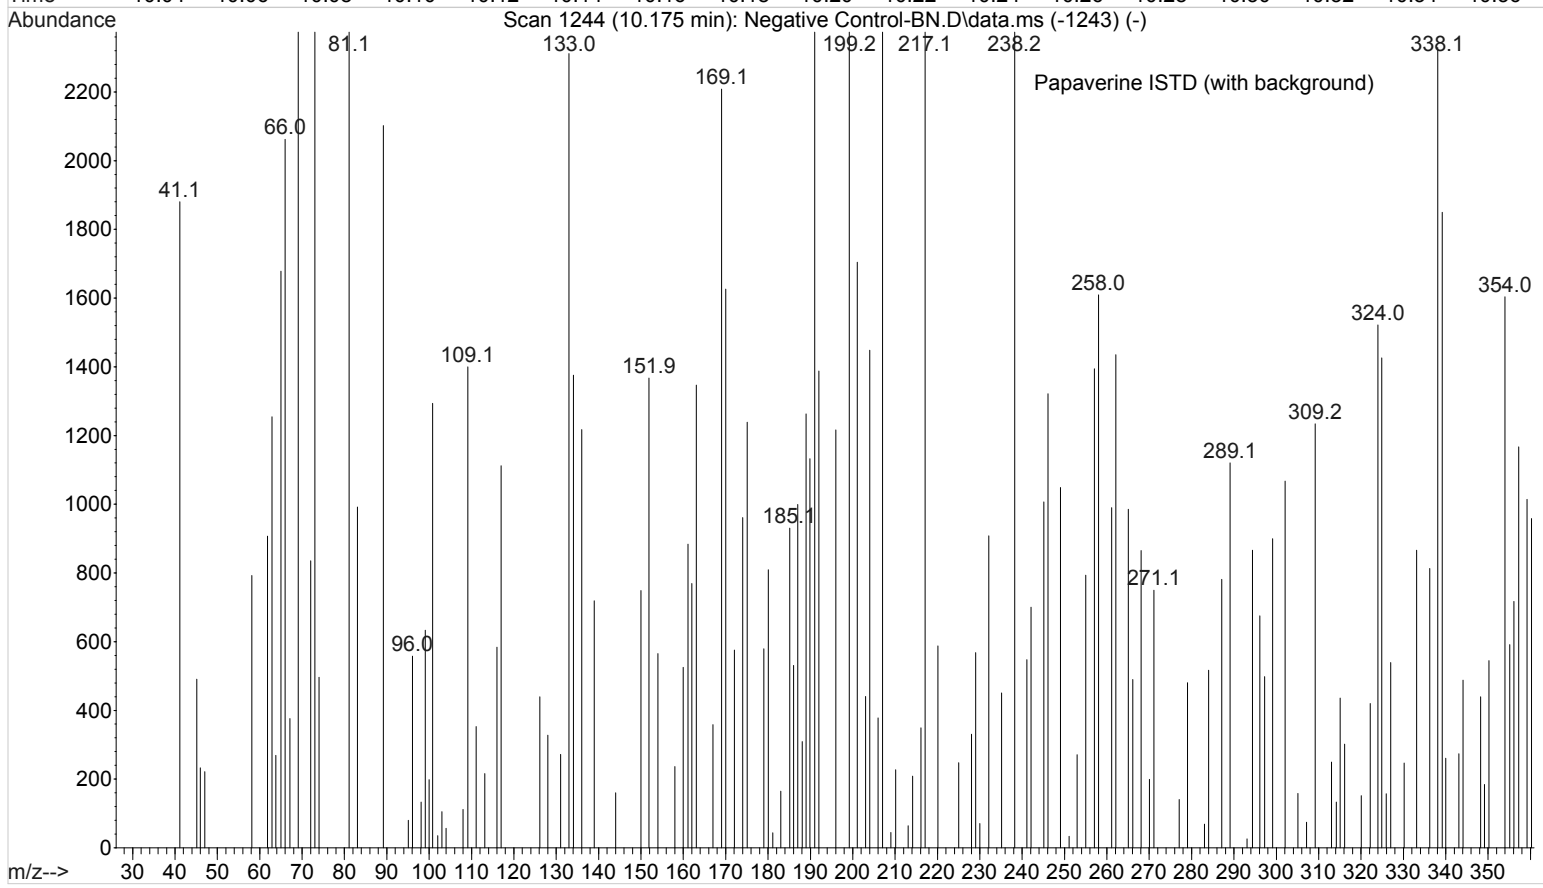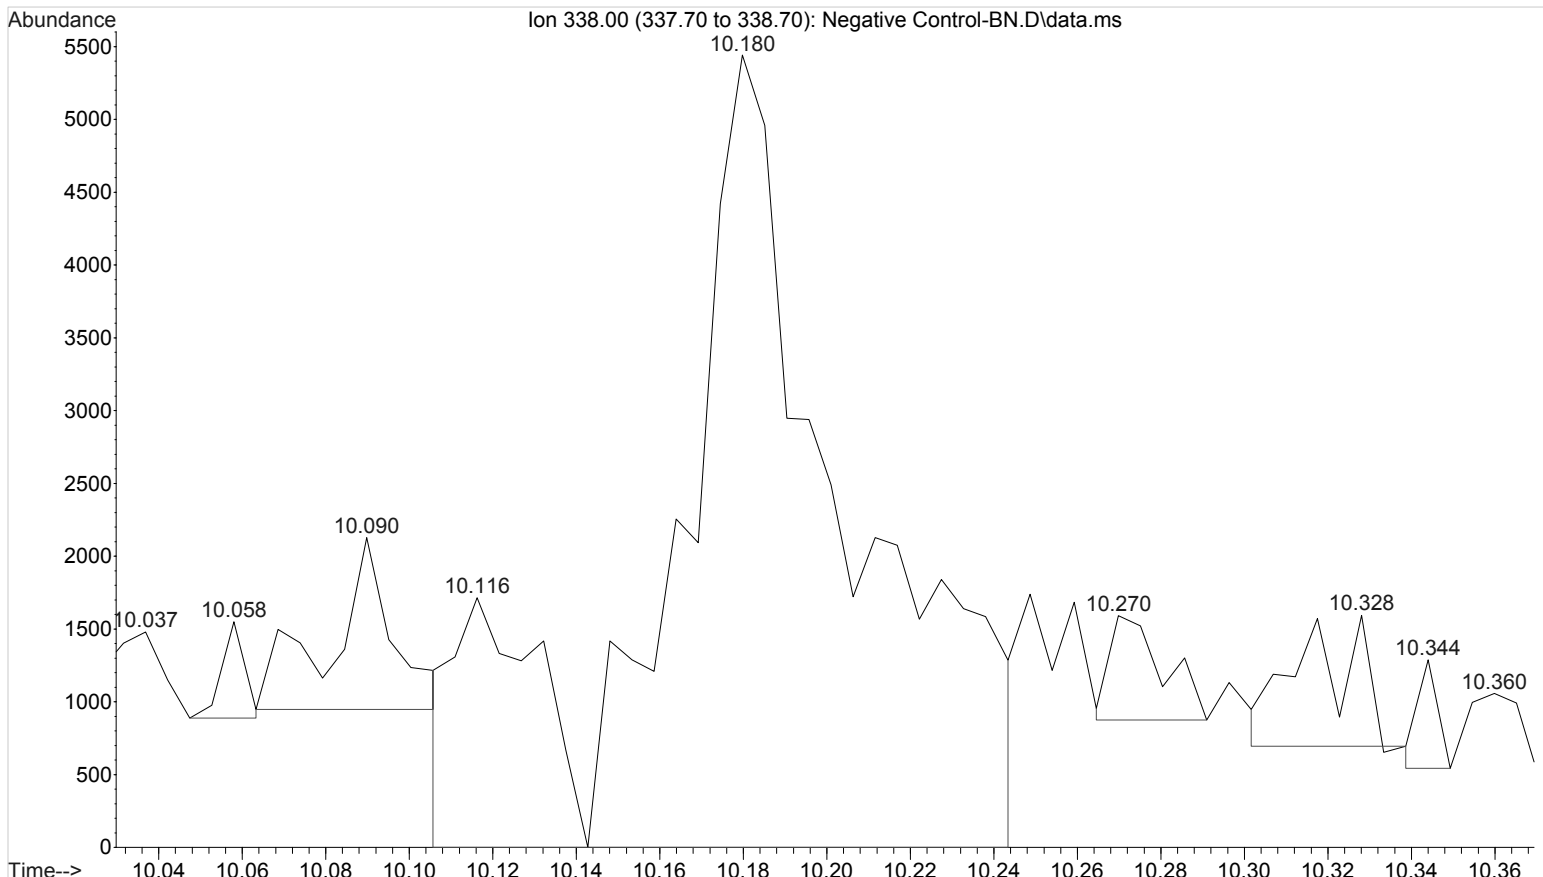



File :I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2017\042817
... \Spiked Positive Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 28 Apr 2017 11:48 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111616

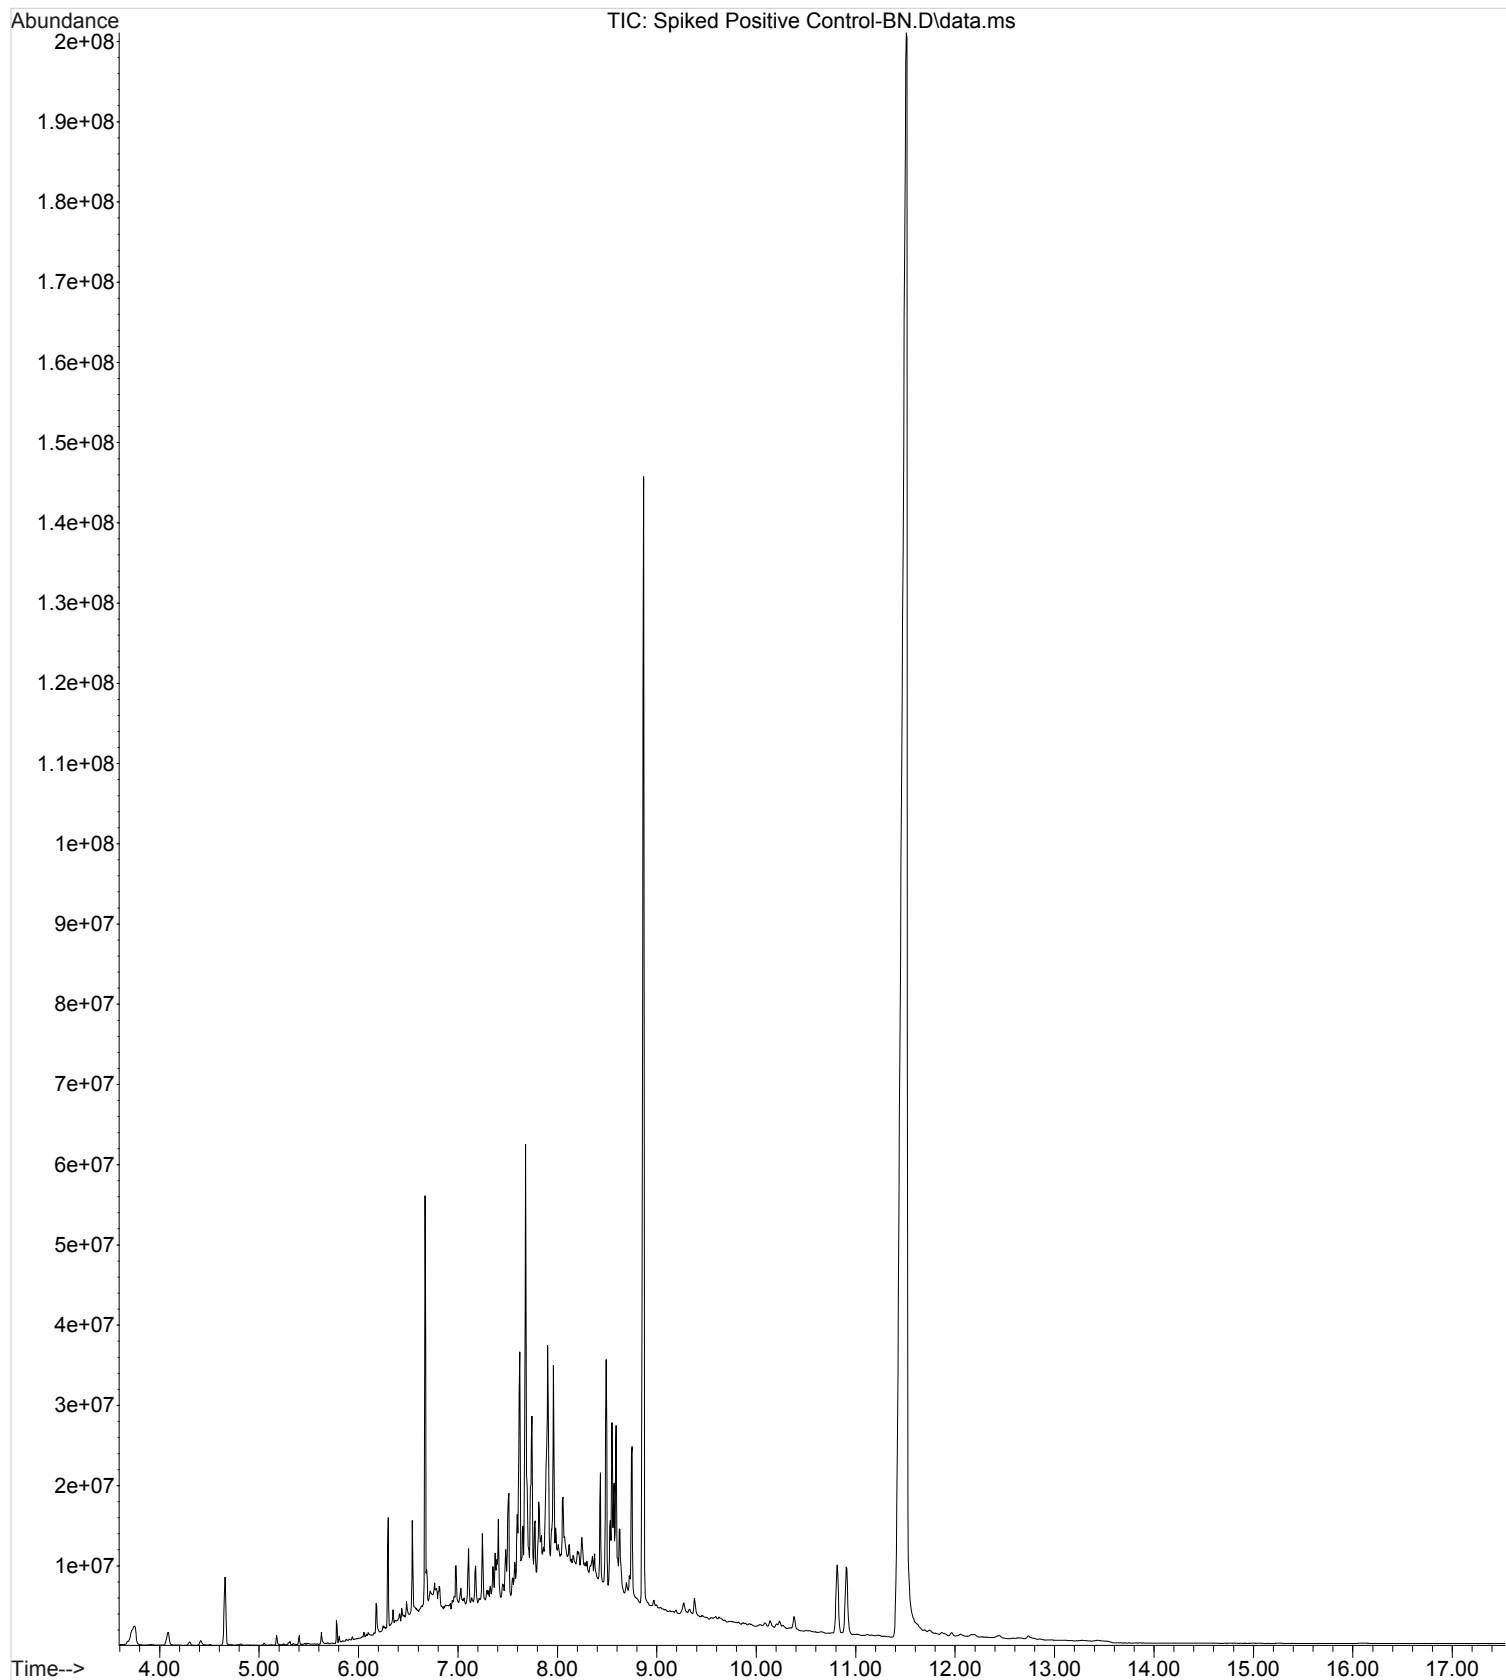

File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2017\042817
... \Spiked Positive Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 28 Apr 2017 11:48 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111616

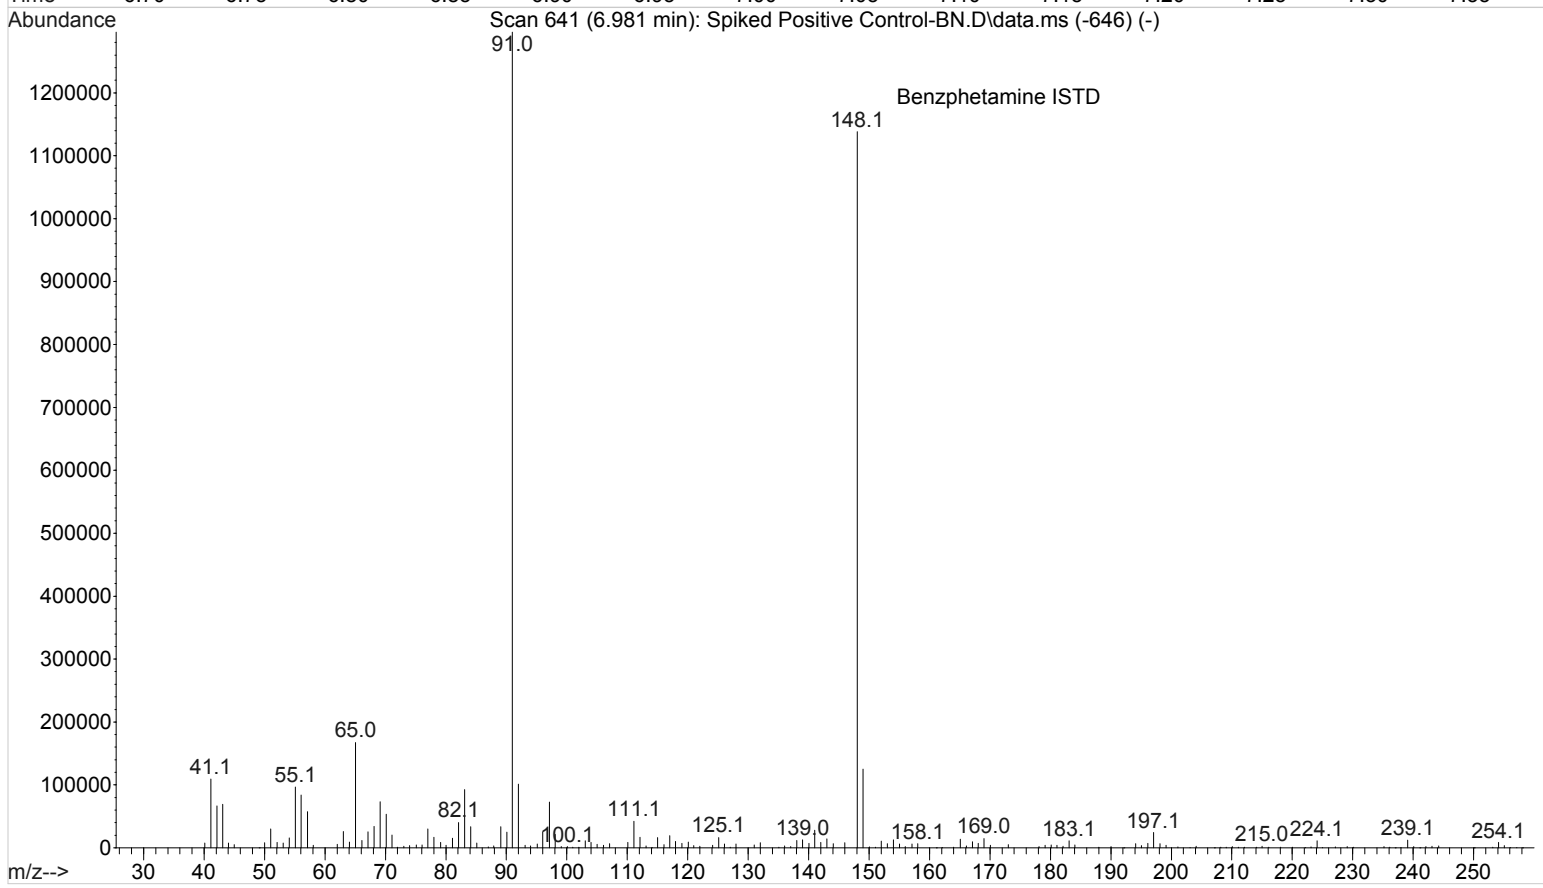
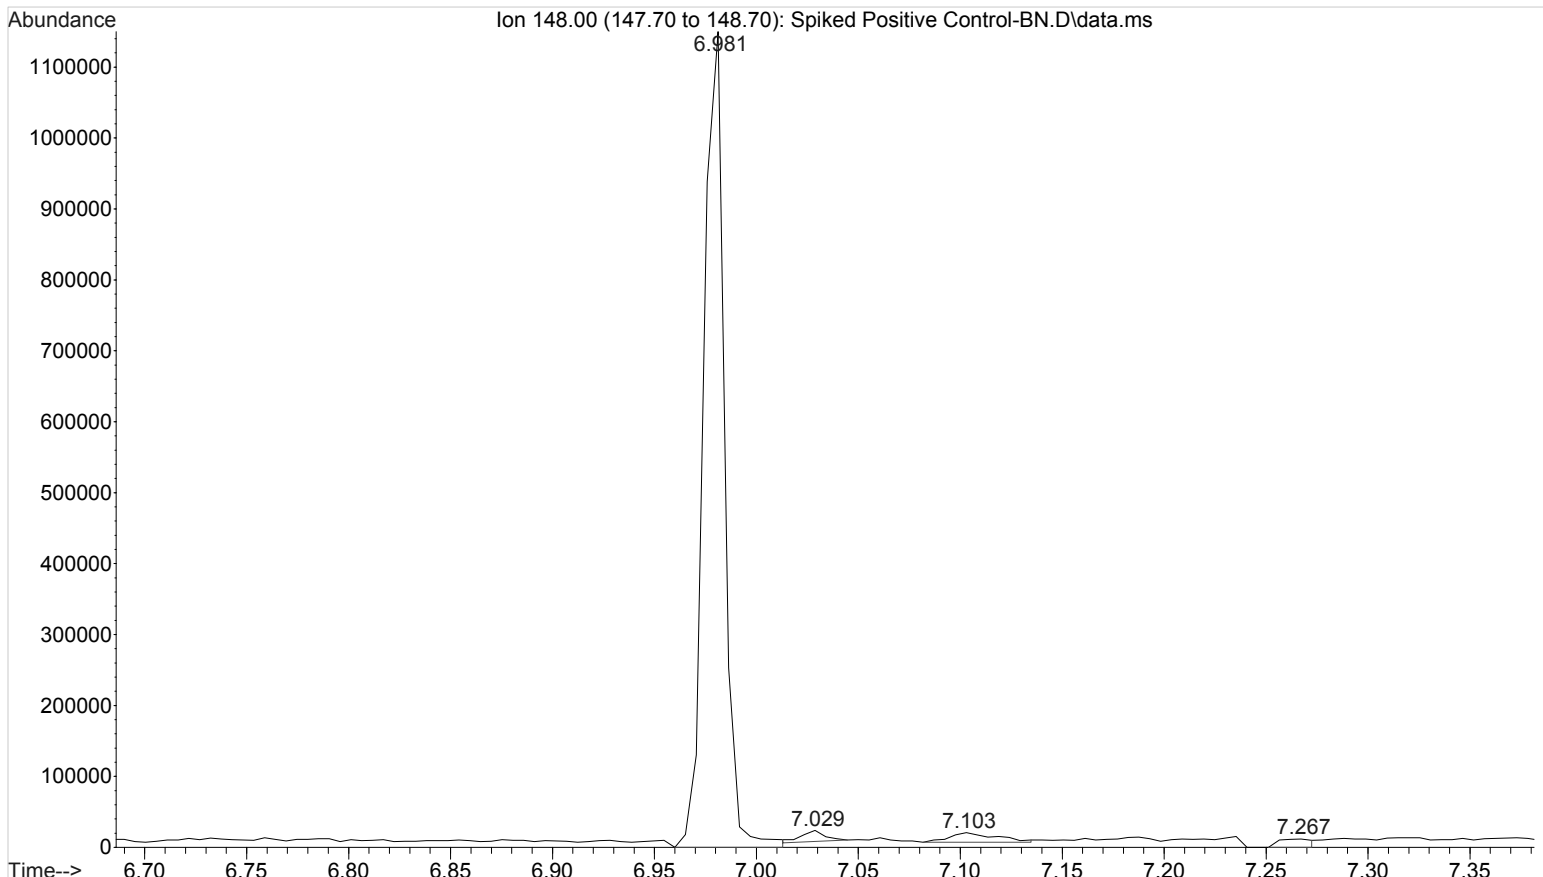


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2017\042817
... \Spiked Positive Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 28 Apr 2017 11:48 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111616

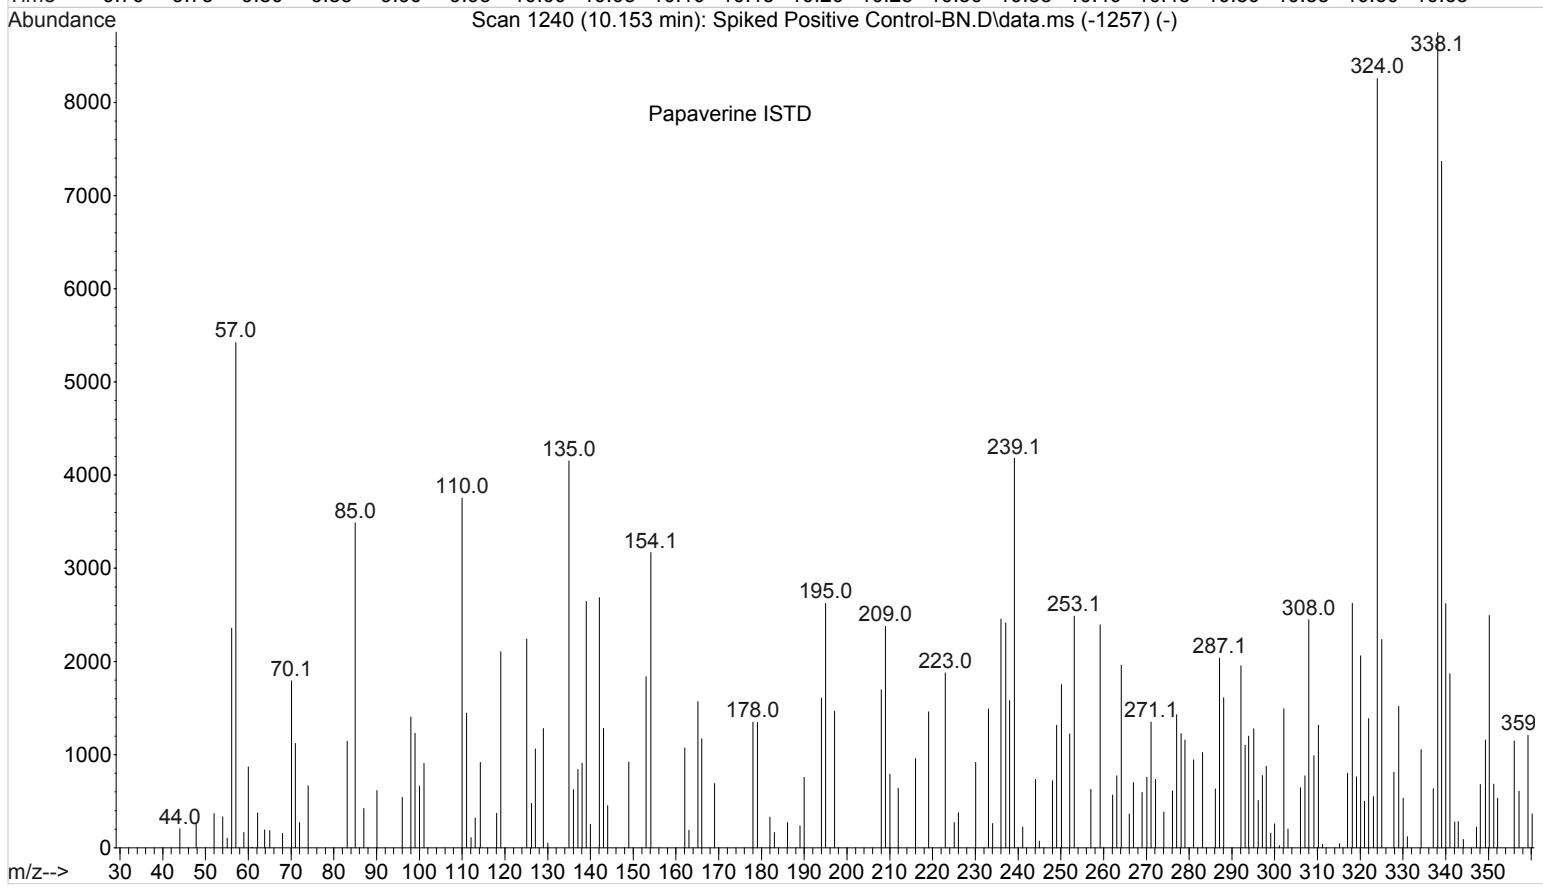
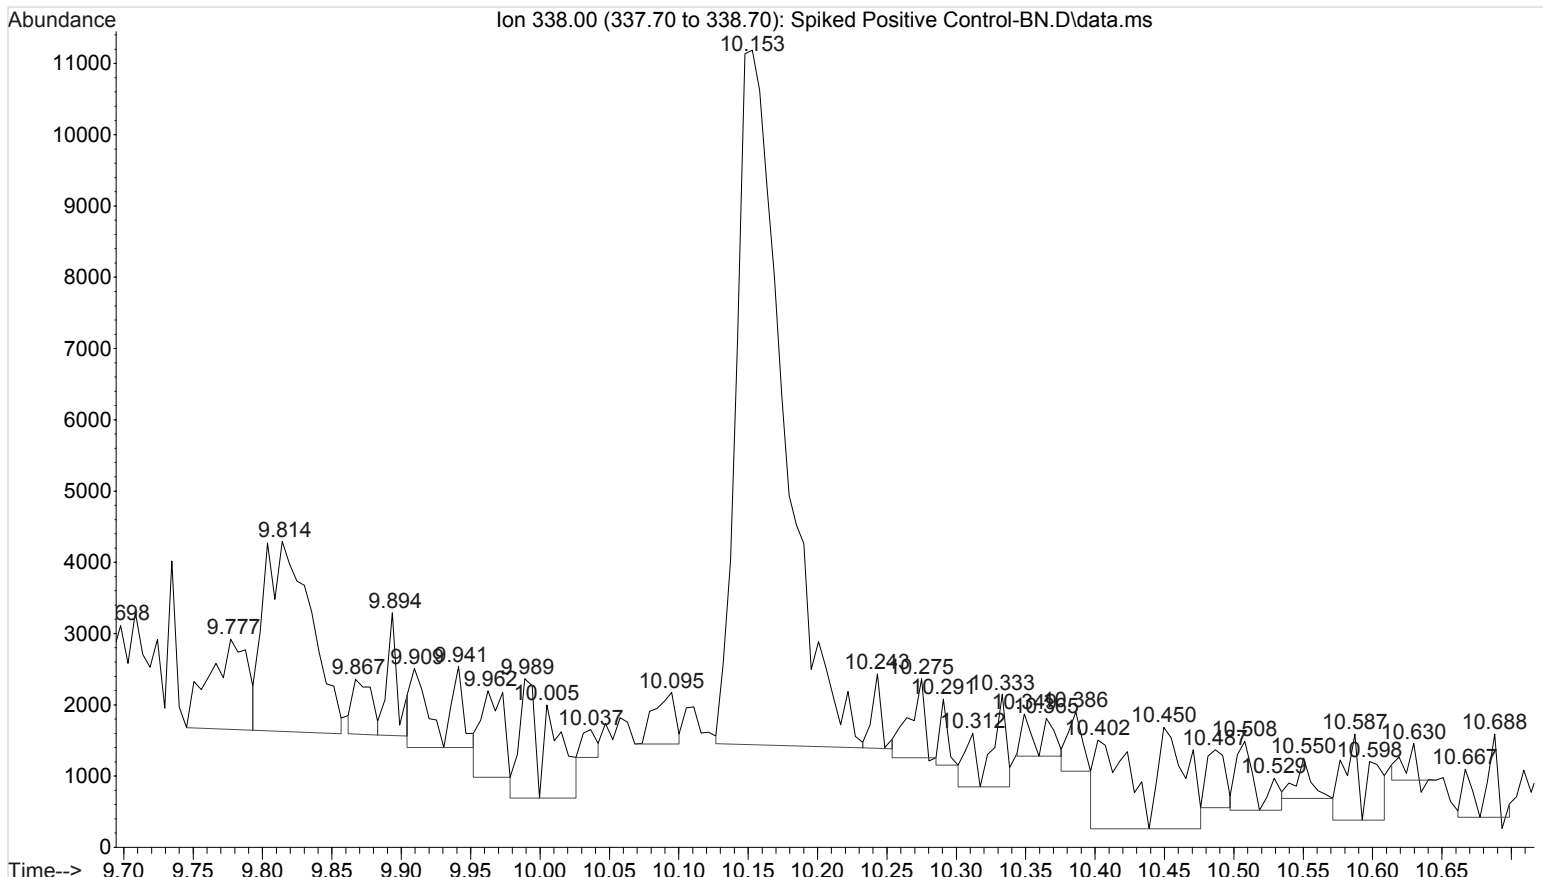


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2017\042817
... \Spiked Positive Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 28 Apr 2017 11:48 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111616

CS

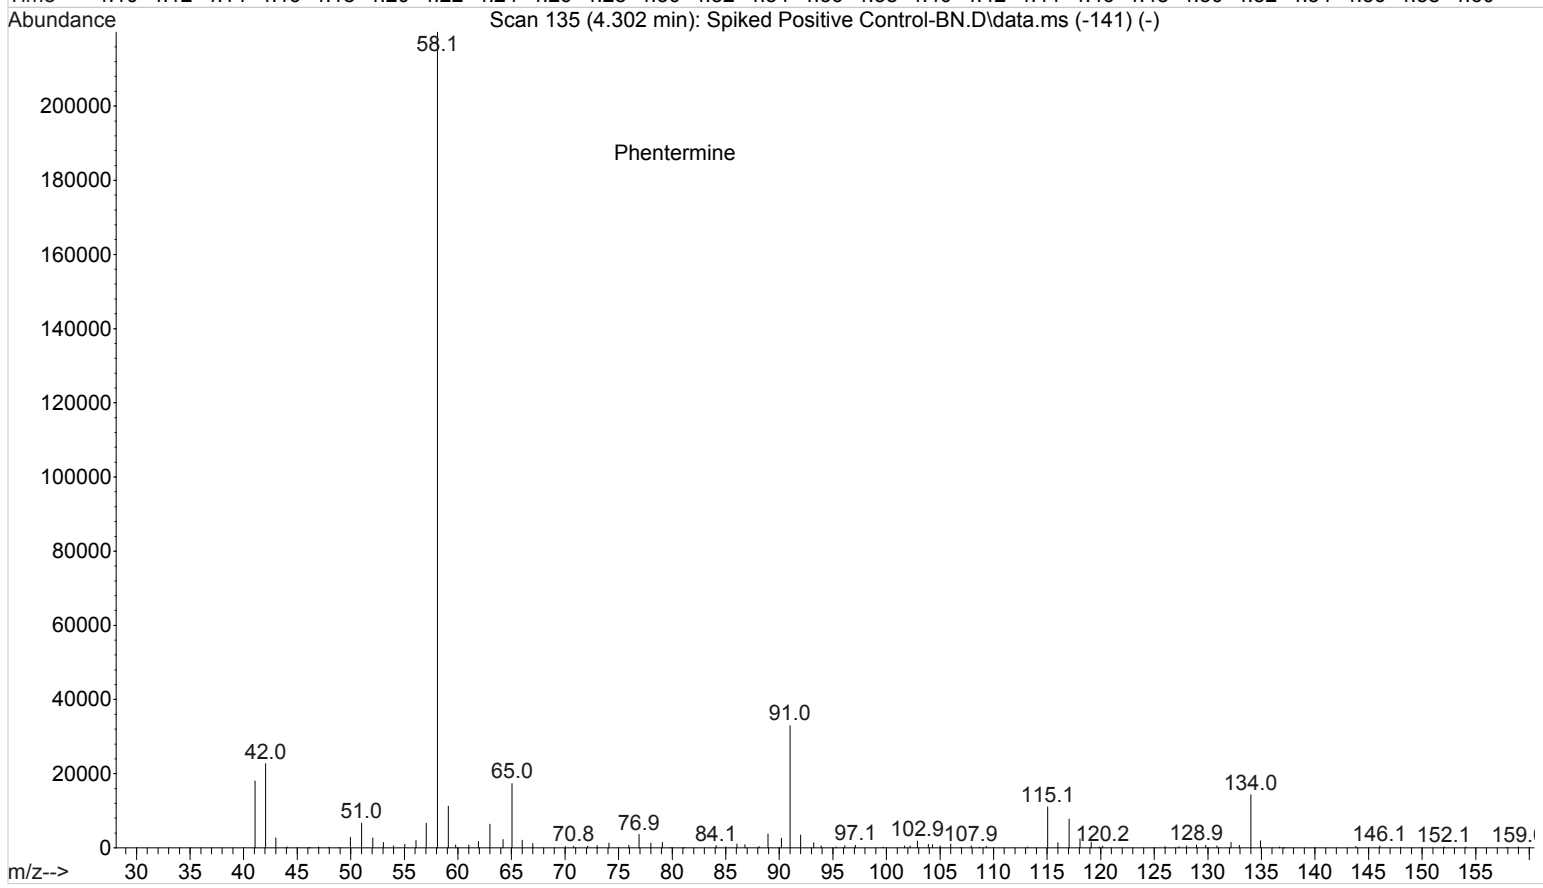
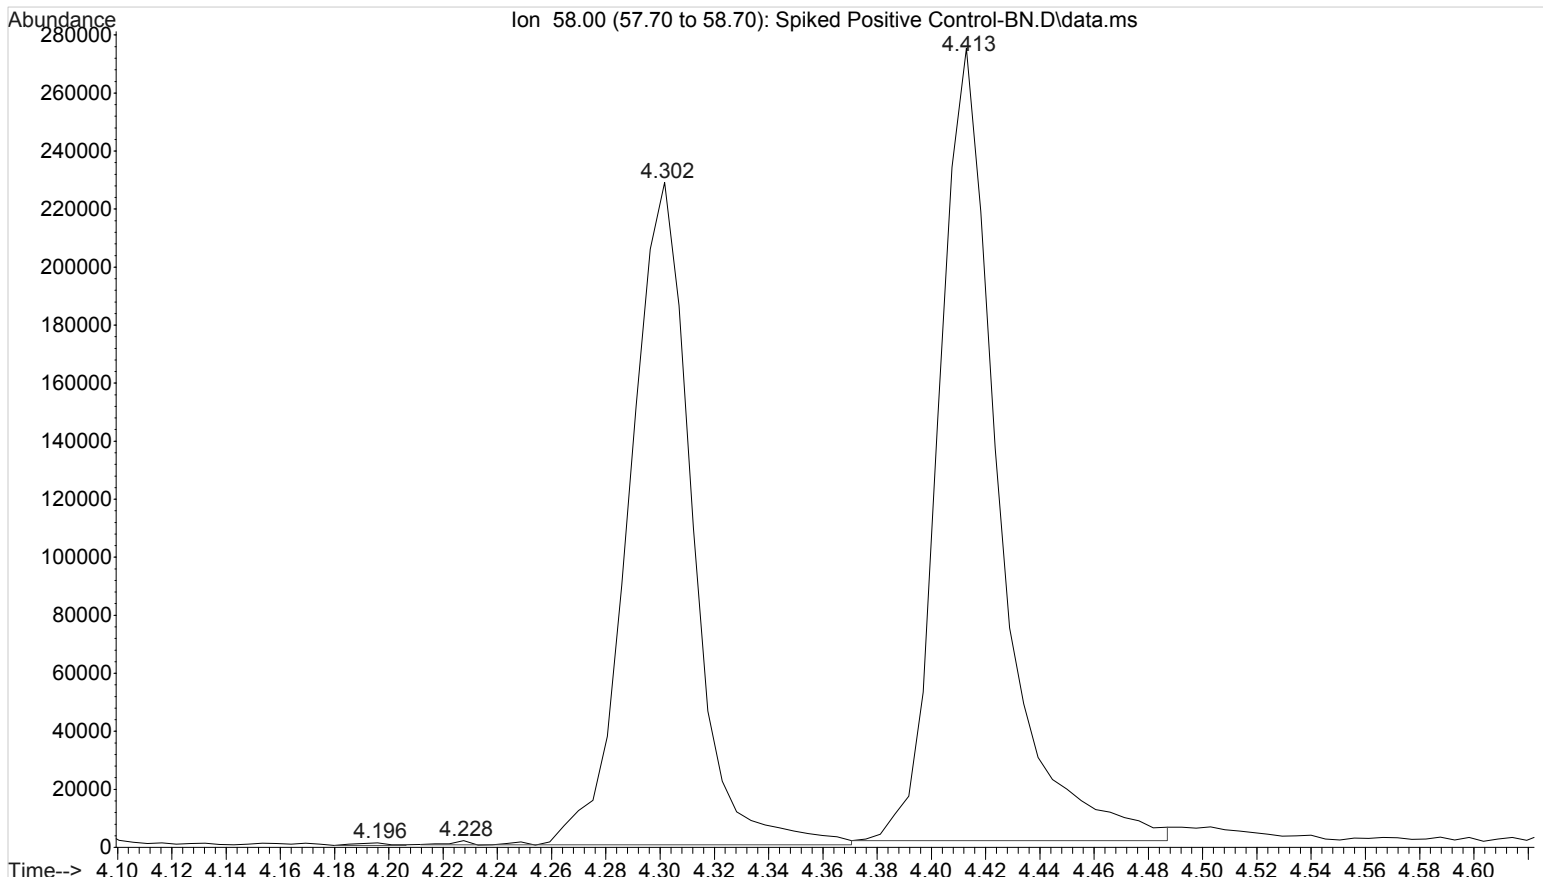


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2017\042817
... \Spiked Positive Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 28 Apr 2017 11:48 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111616

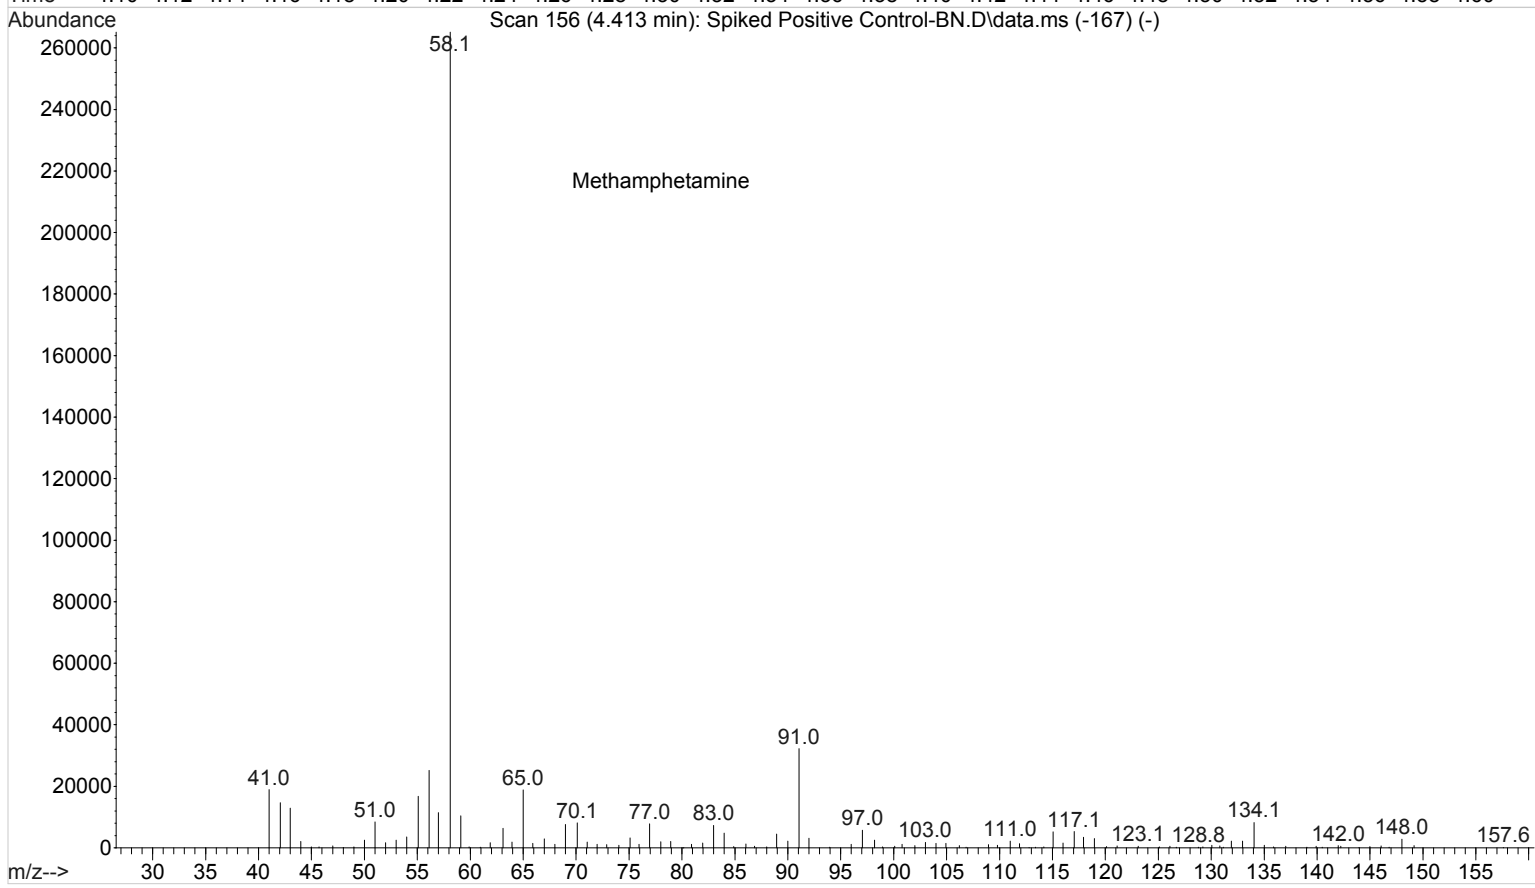
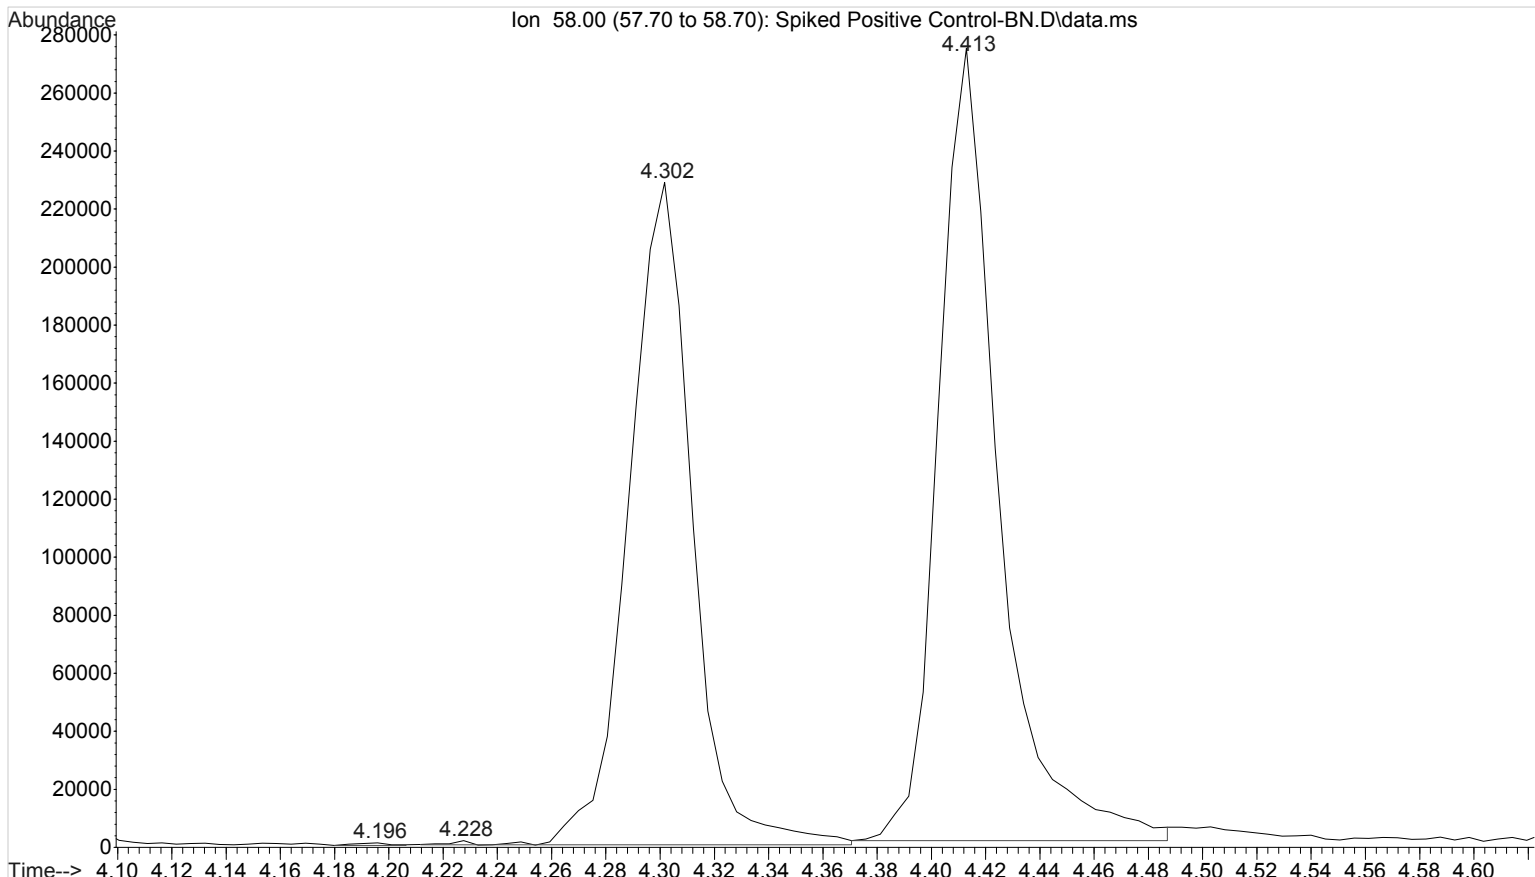


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2017\042817
... \Spiked Positive Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 28 Apr 2017 11:48 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111616

5

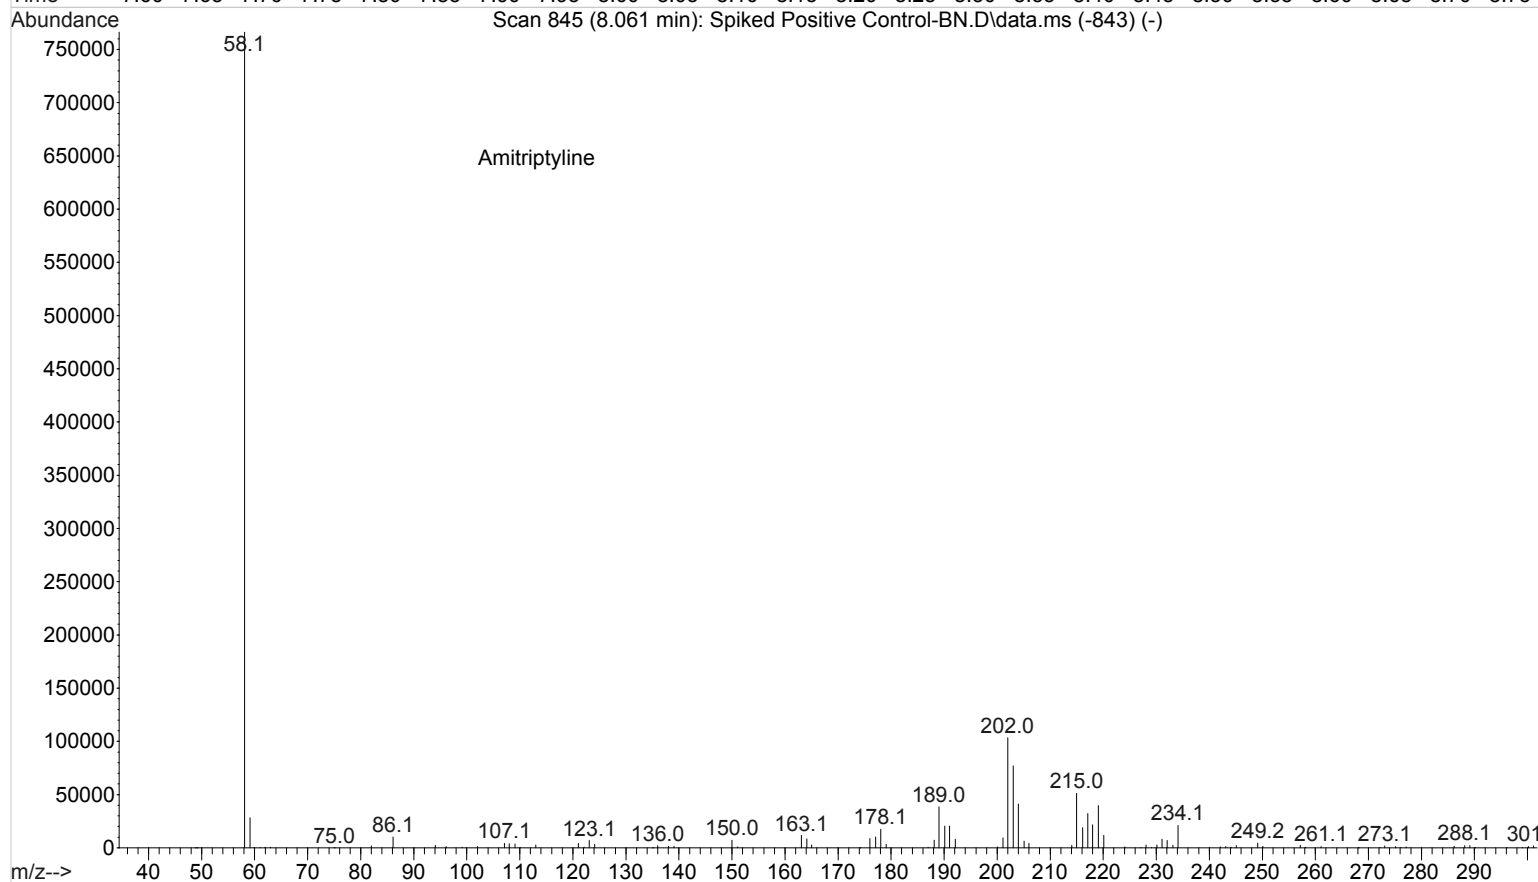
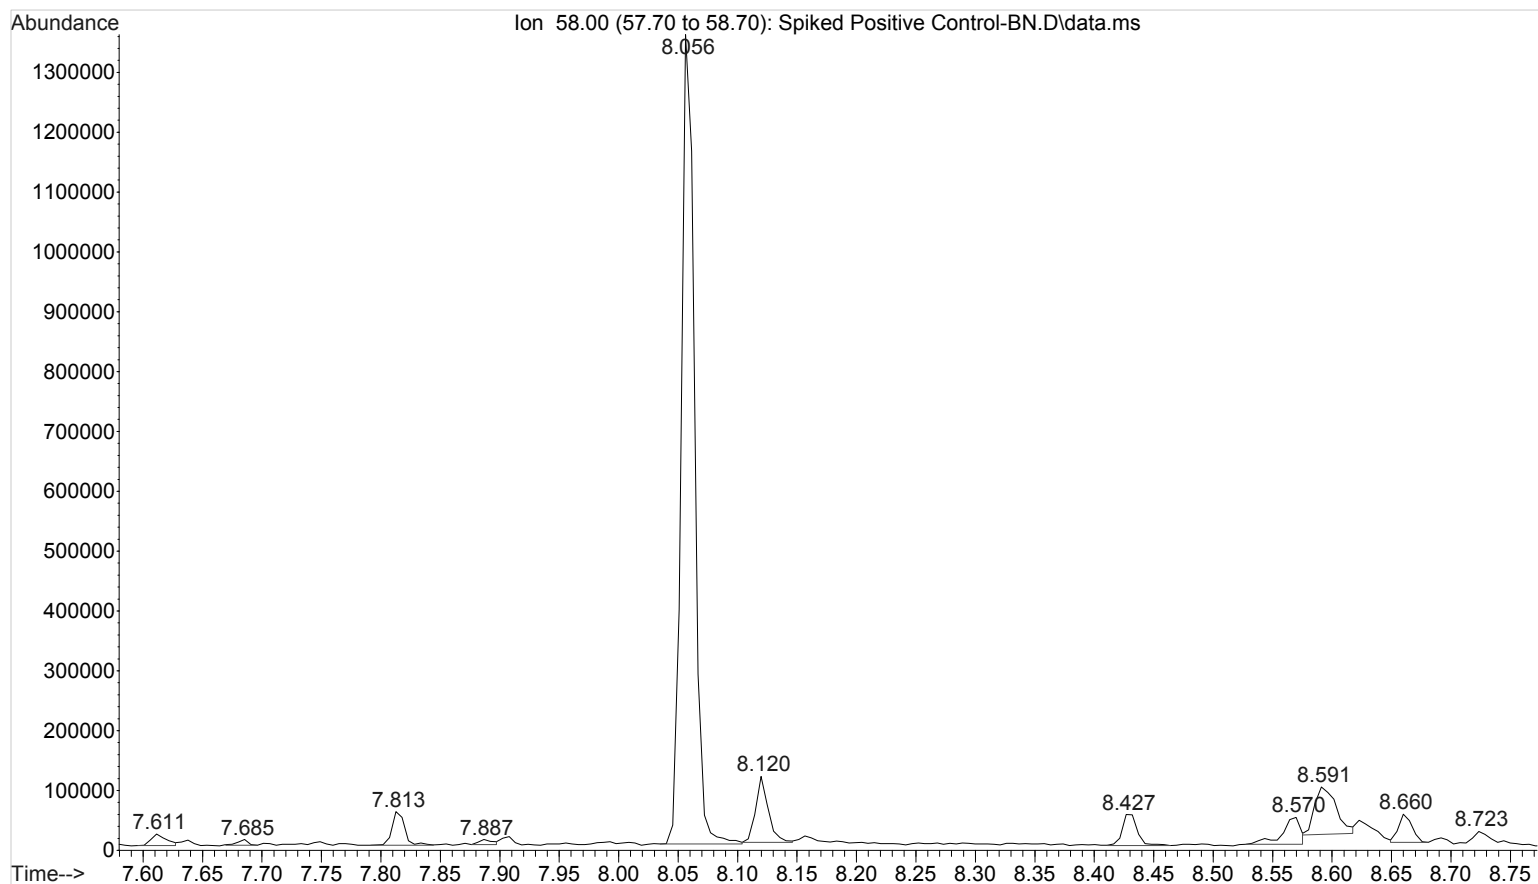


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2017\042817
... \Spiked Positive Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 28 Apr 2017 11:48 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111616

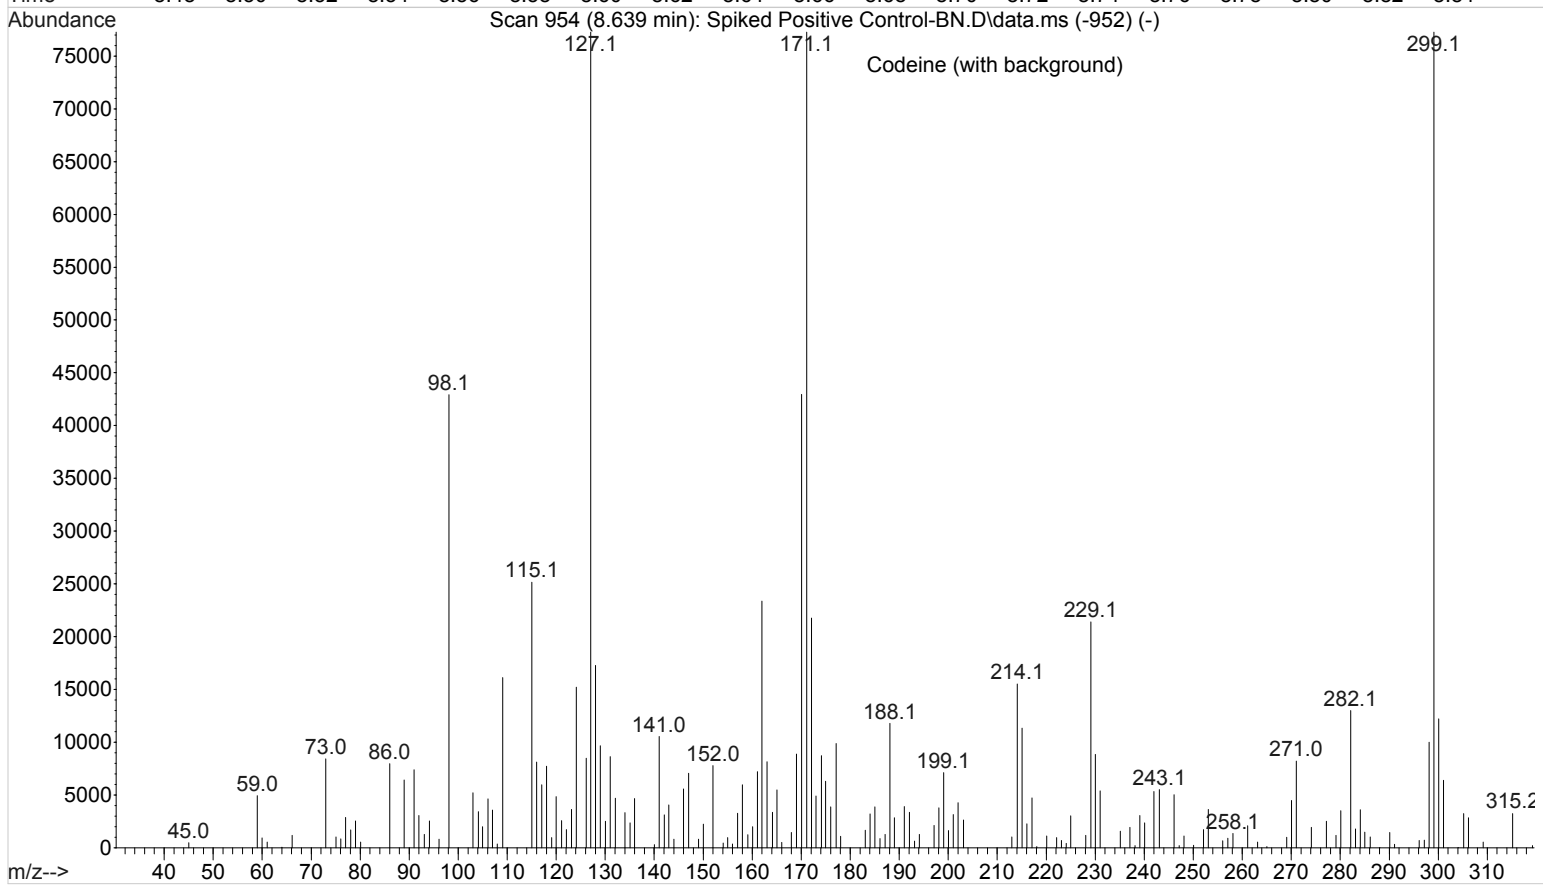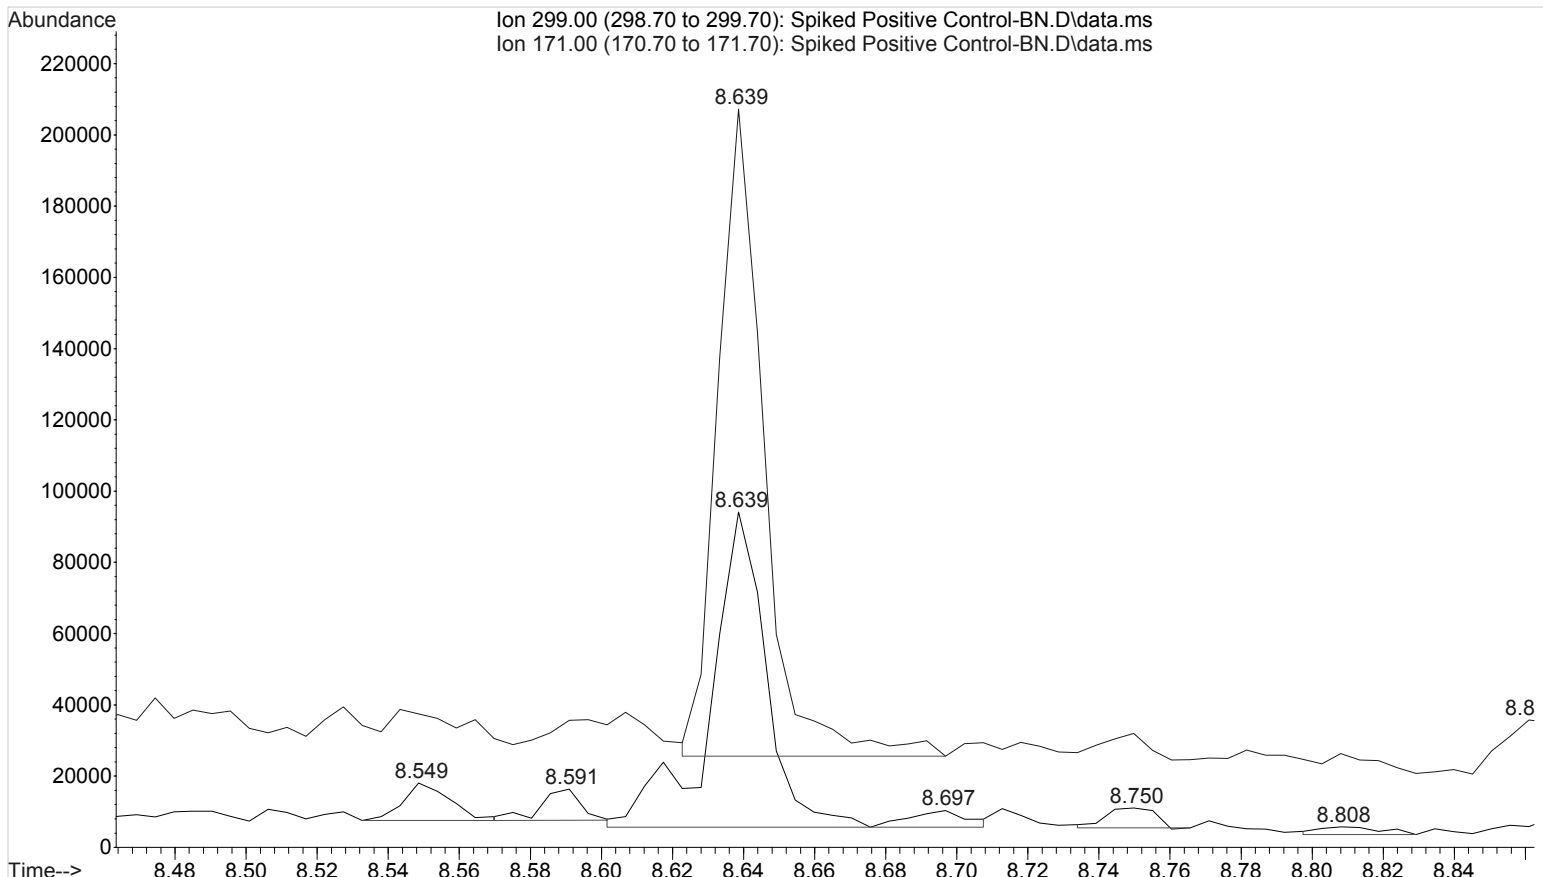


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2017\042817
... \Spiked Positive Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 28 Apr 2017 11:48 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111616

CS

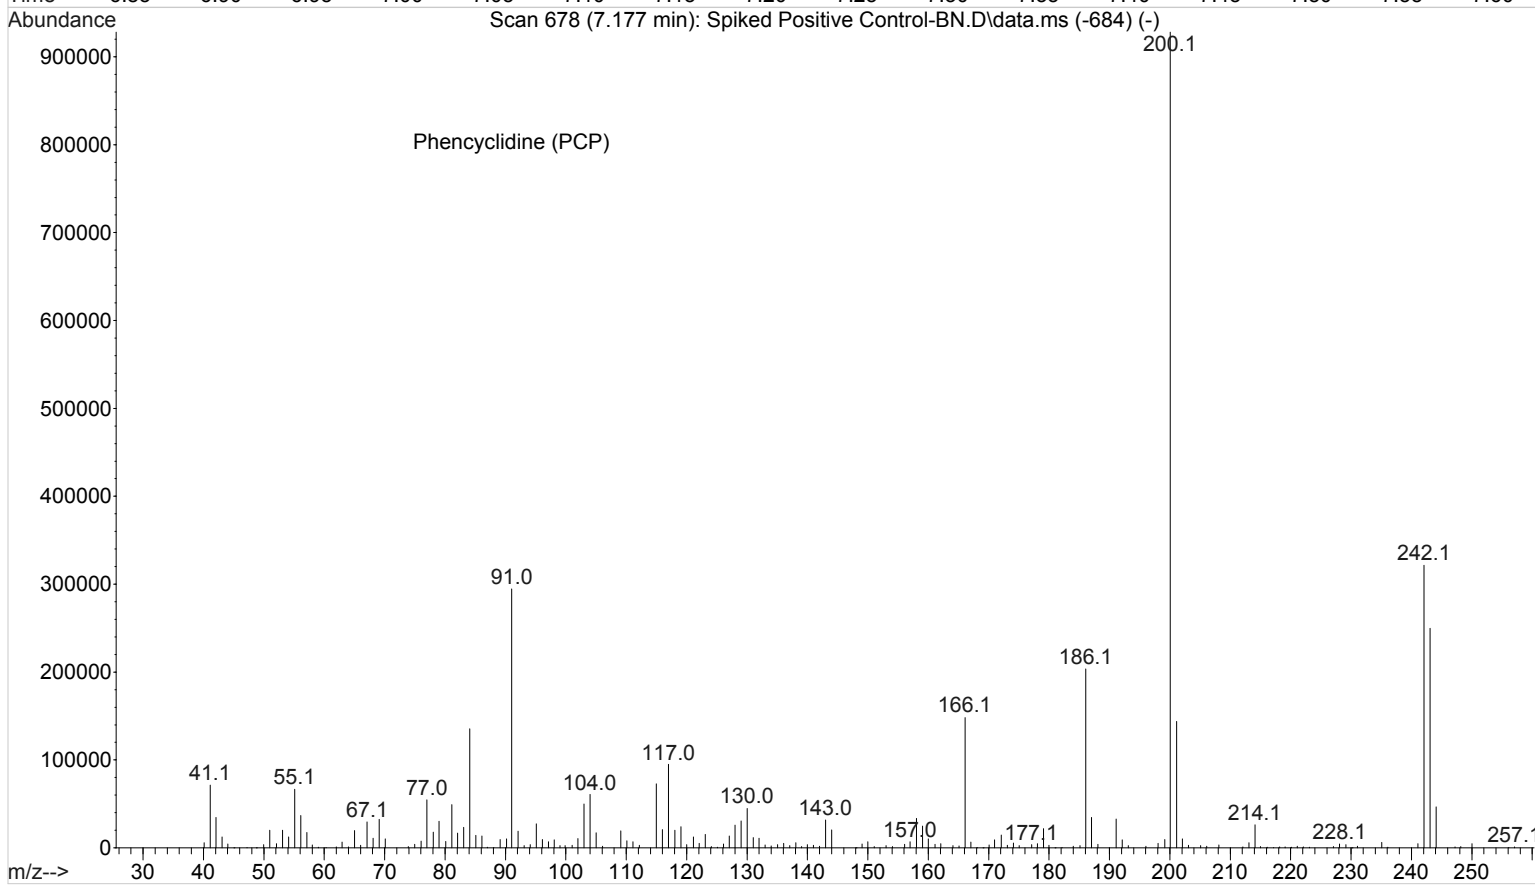
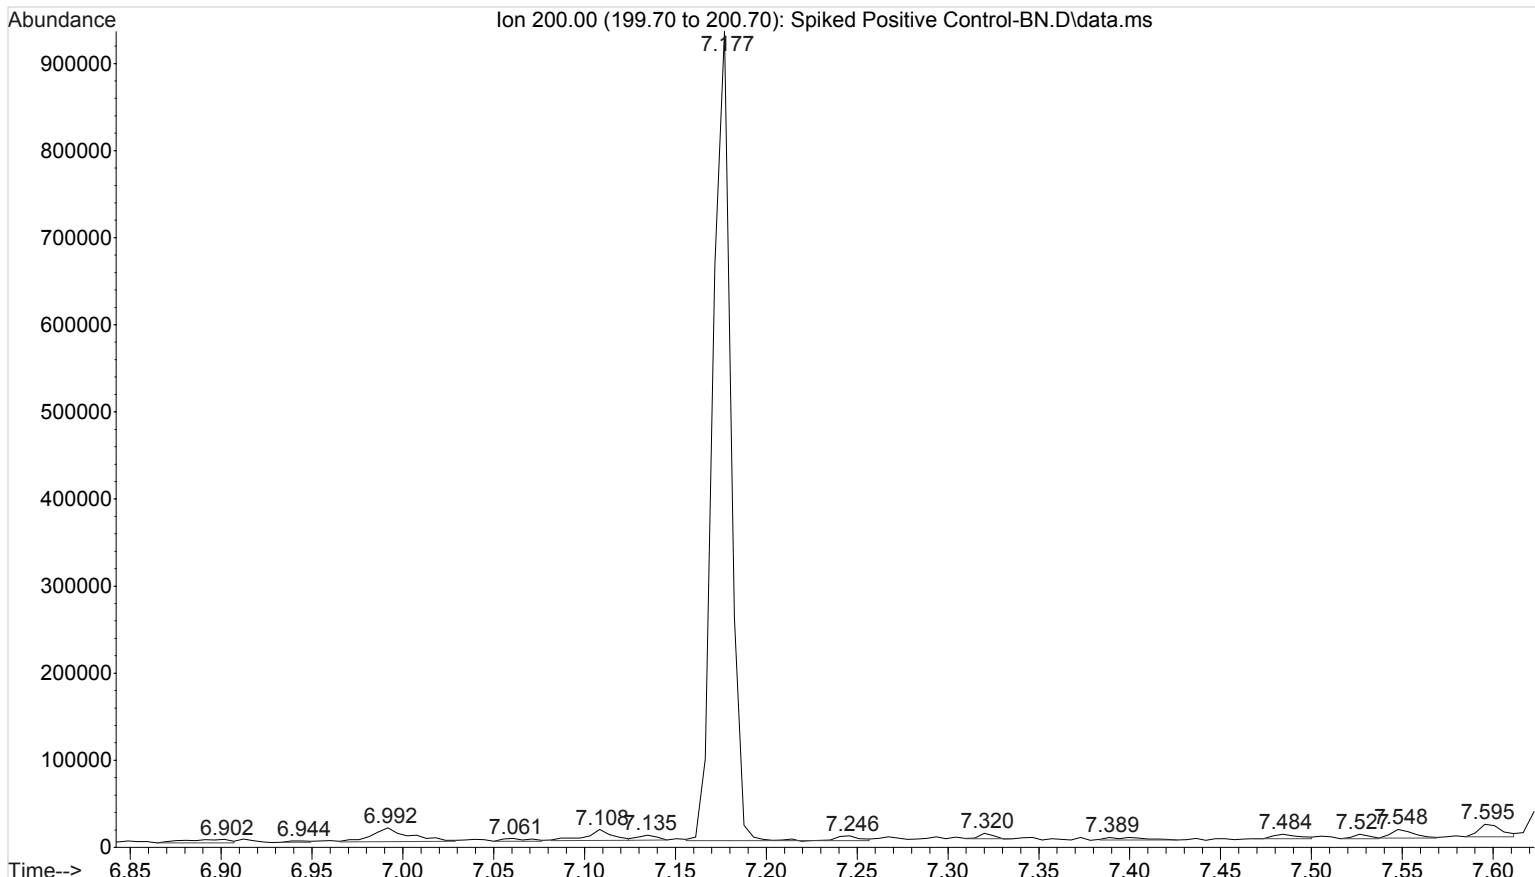


File :I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2017\042817
... \Negative Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 28 Apr 2017 11:25 using AcqMethod BNSB120510.M
Sample Name: Negative Control - Utak Lot B1013
Misc Info : UTAK B1013


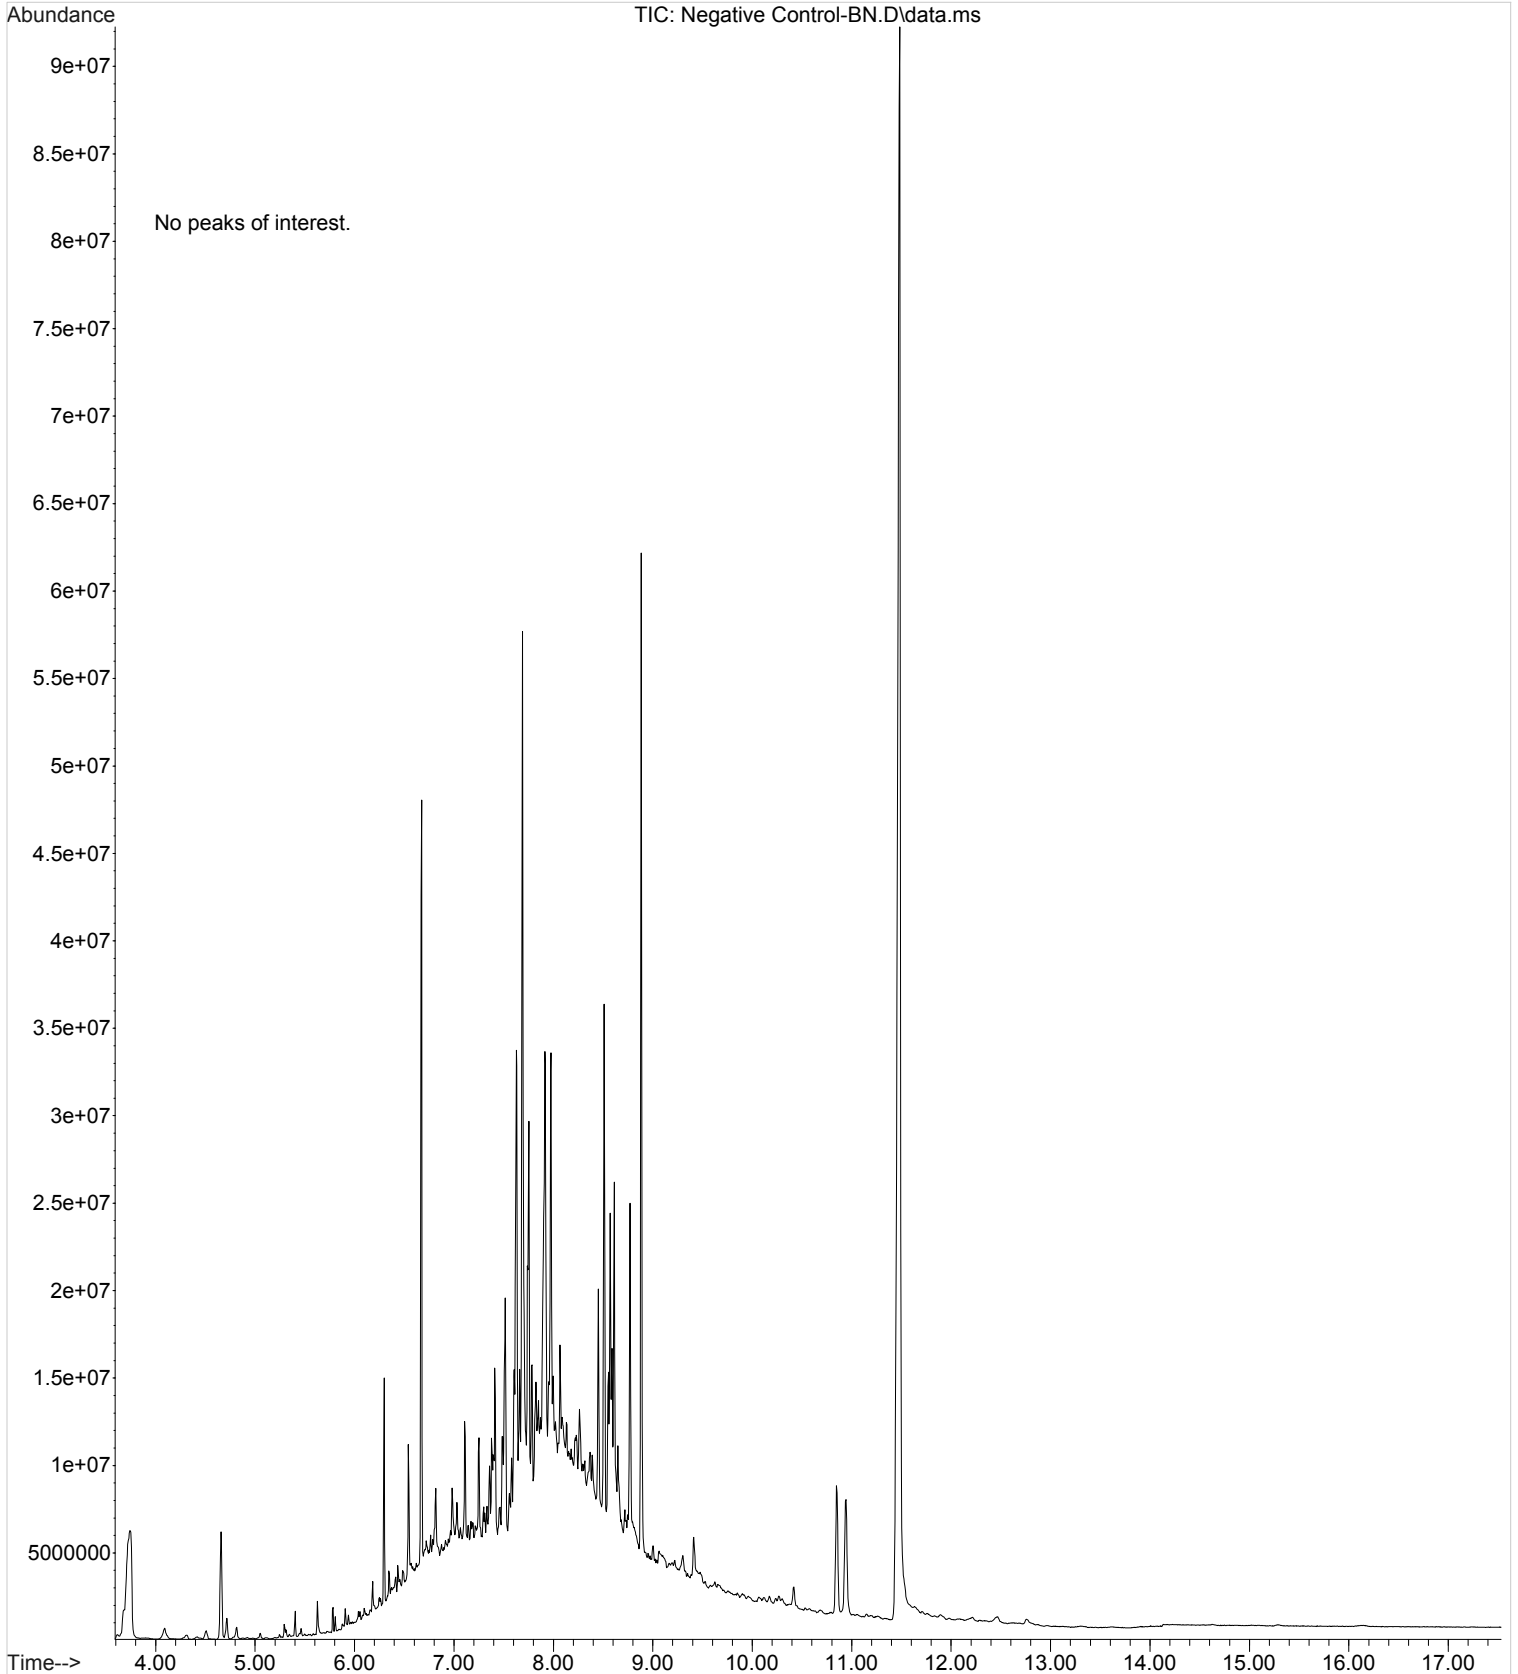


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2017\042817
... \Negative Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 28 Apr 2017 13:07 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Negative Control - Utak Lot B1013
Misc Info : UTAK B1013


CS

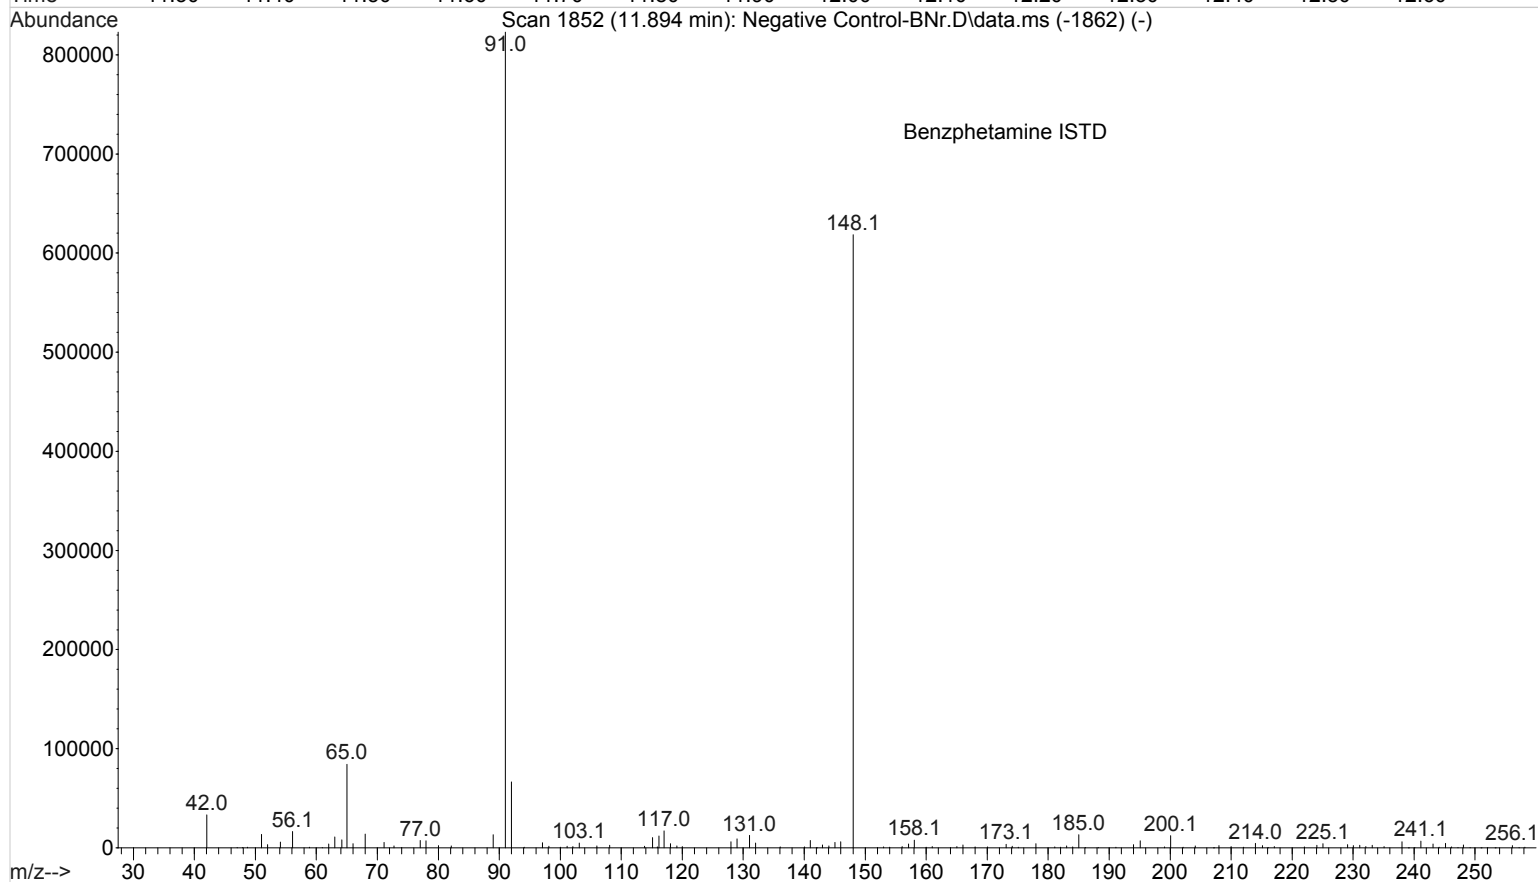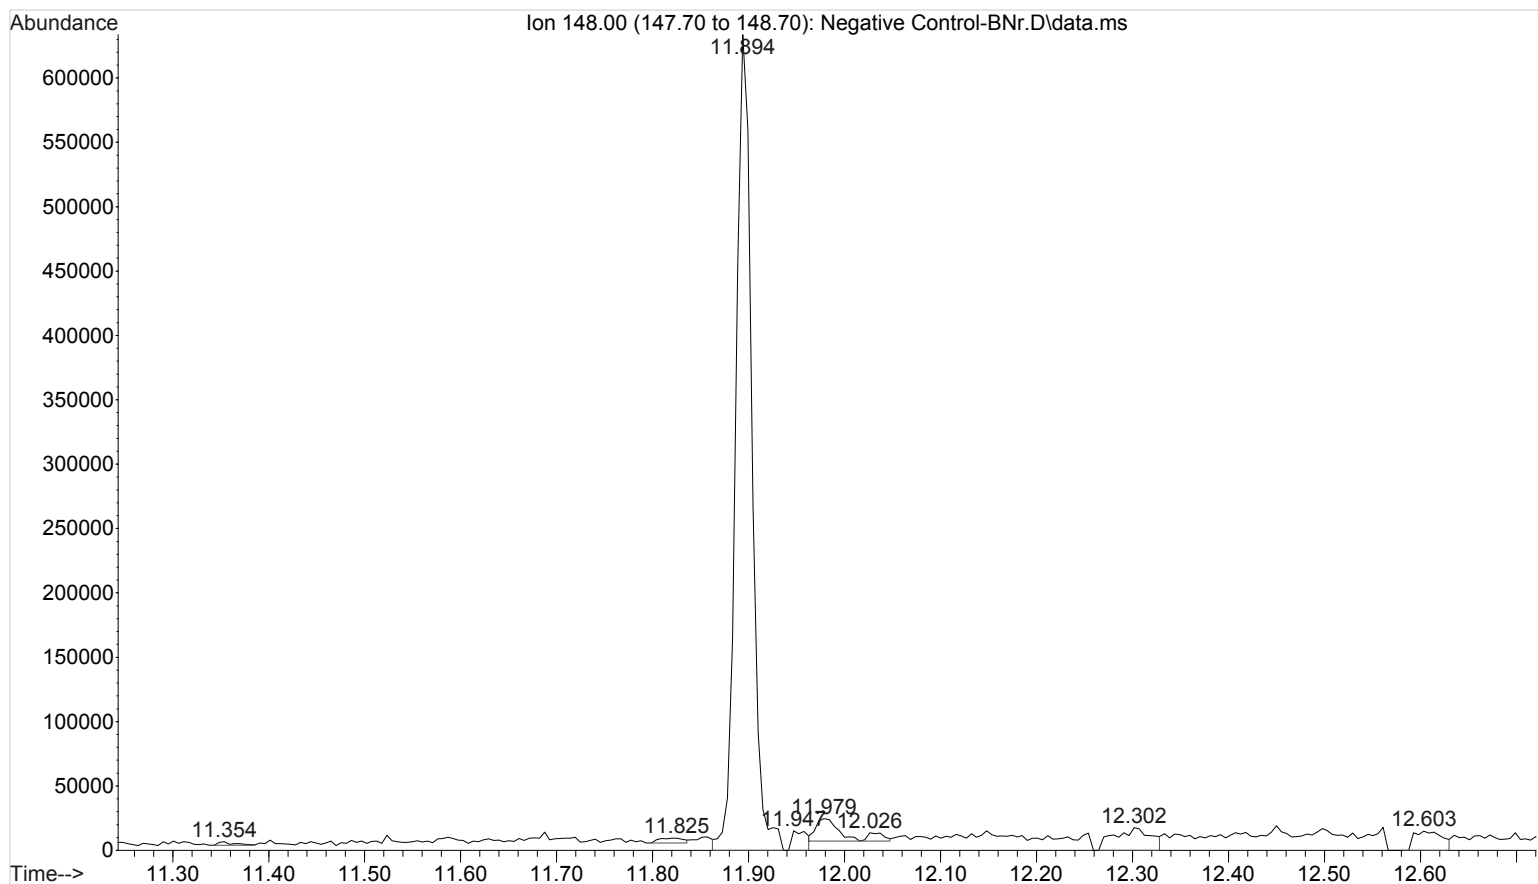



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2017\042817
... \Negative Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 28 Apr 2017 13:07 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Negative Control - Utak Lot B1013
Misc Info : UTAK B1013

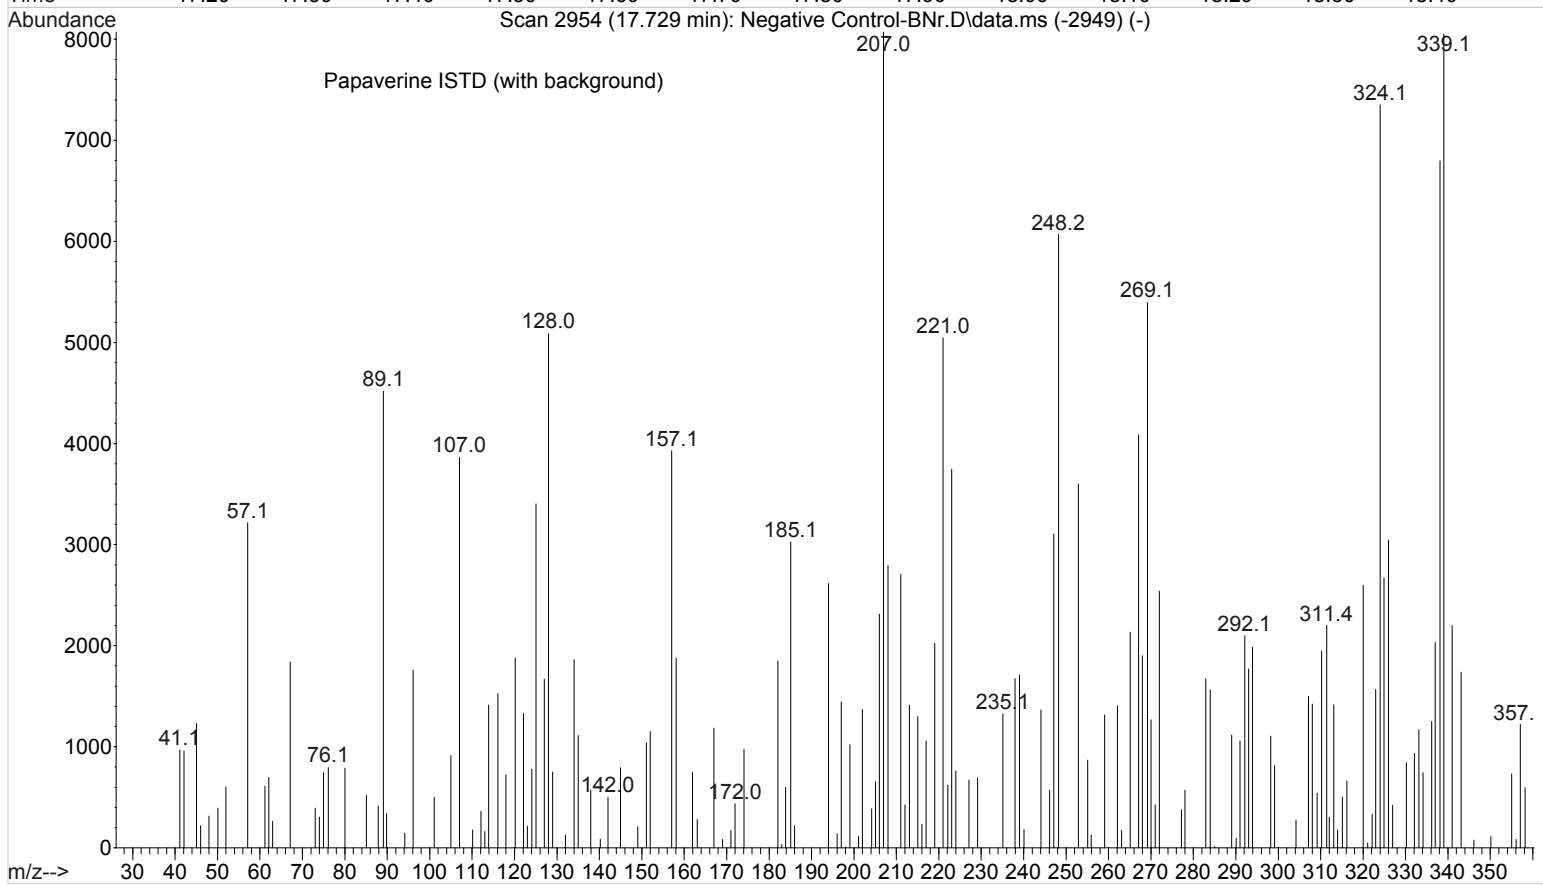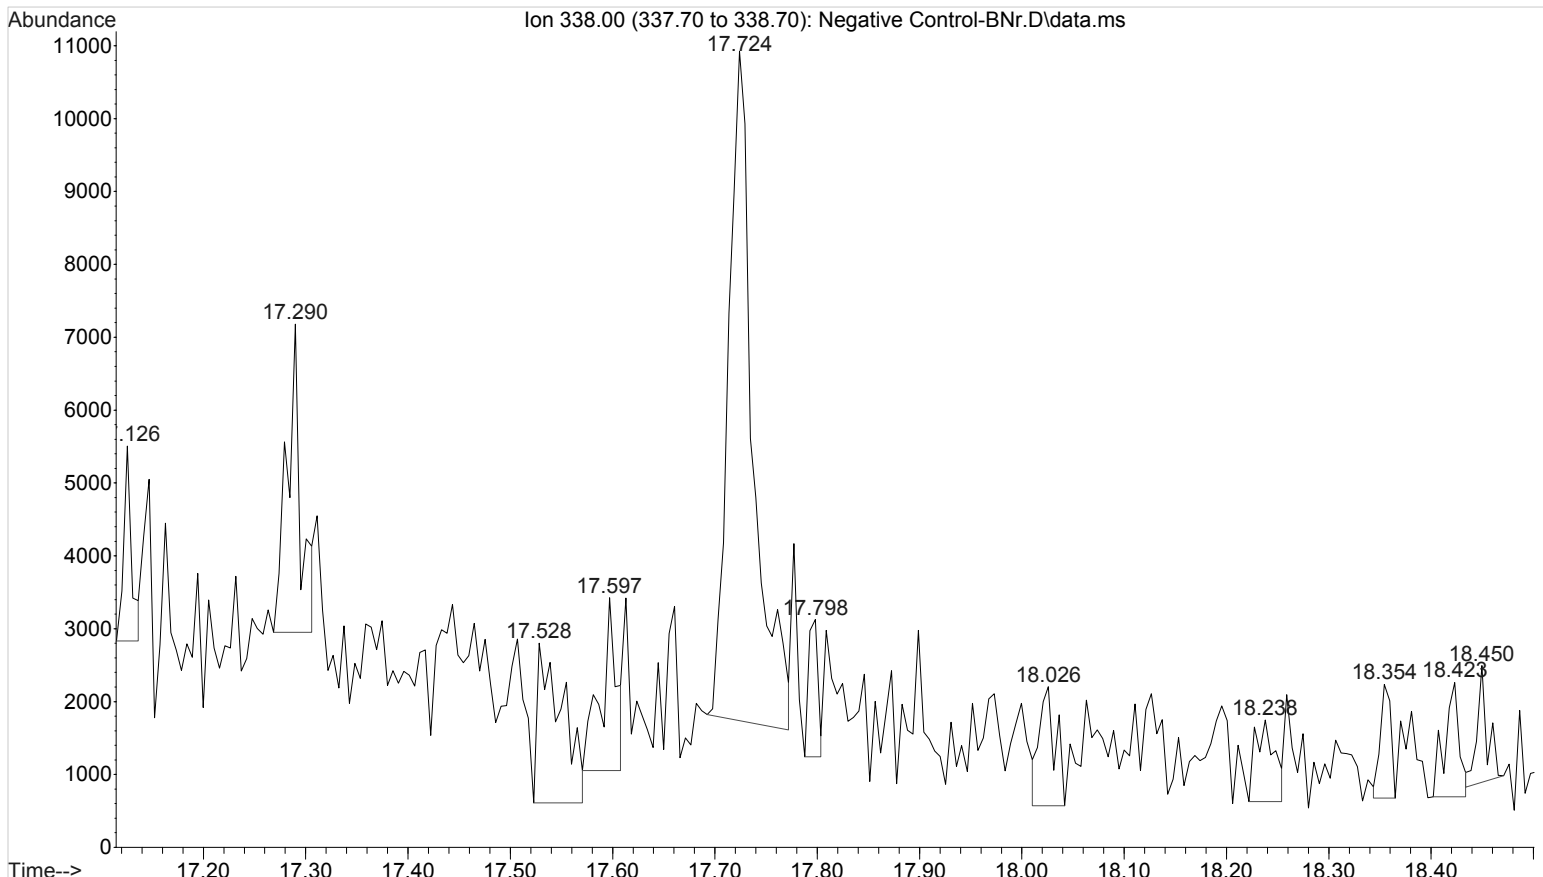



File :I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2017\042817
... \Spiked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 28 Apr 2017 13:41 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111616

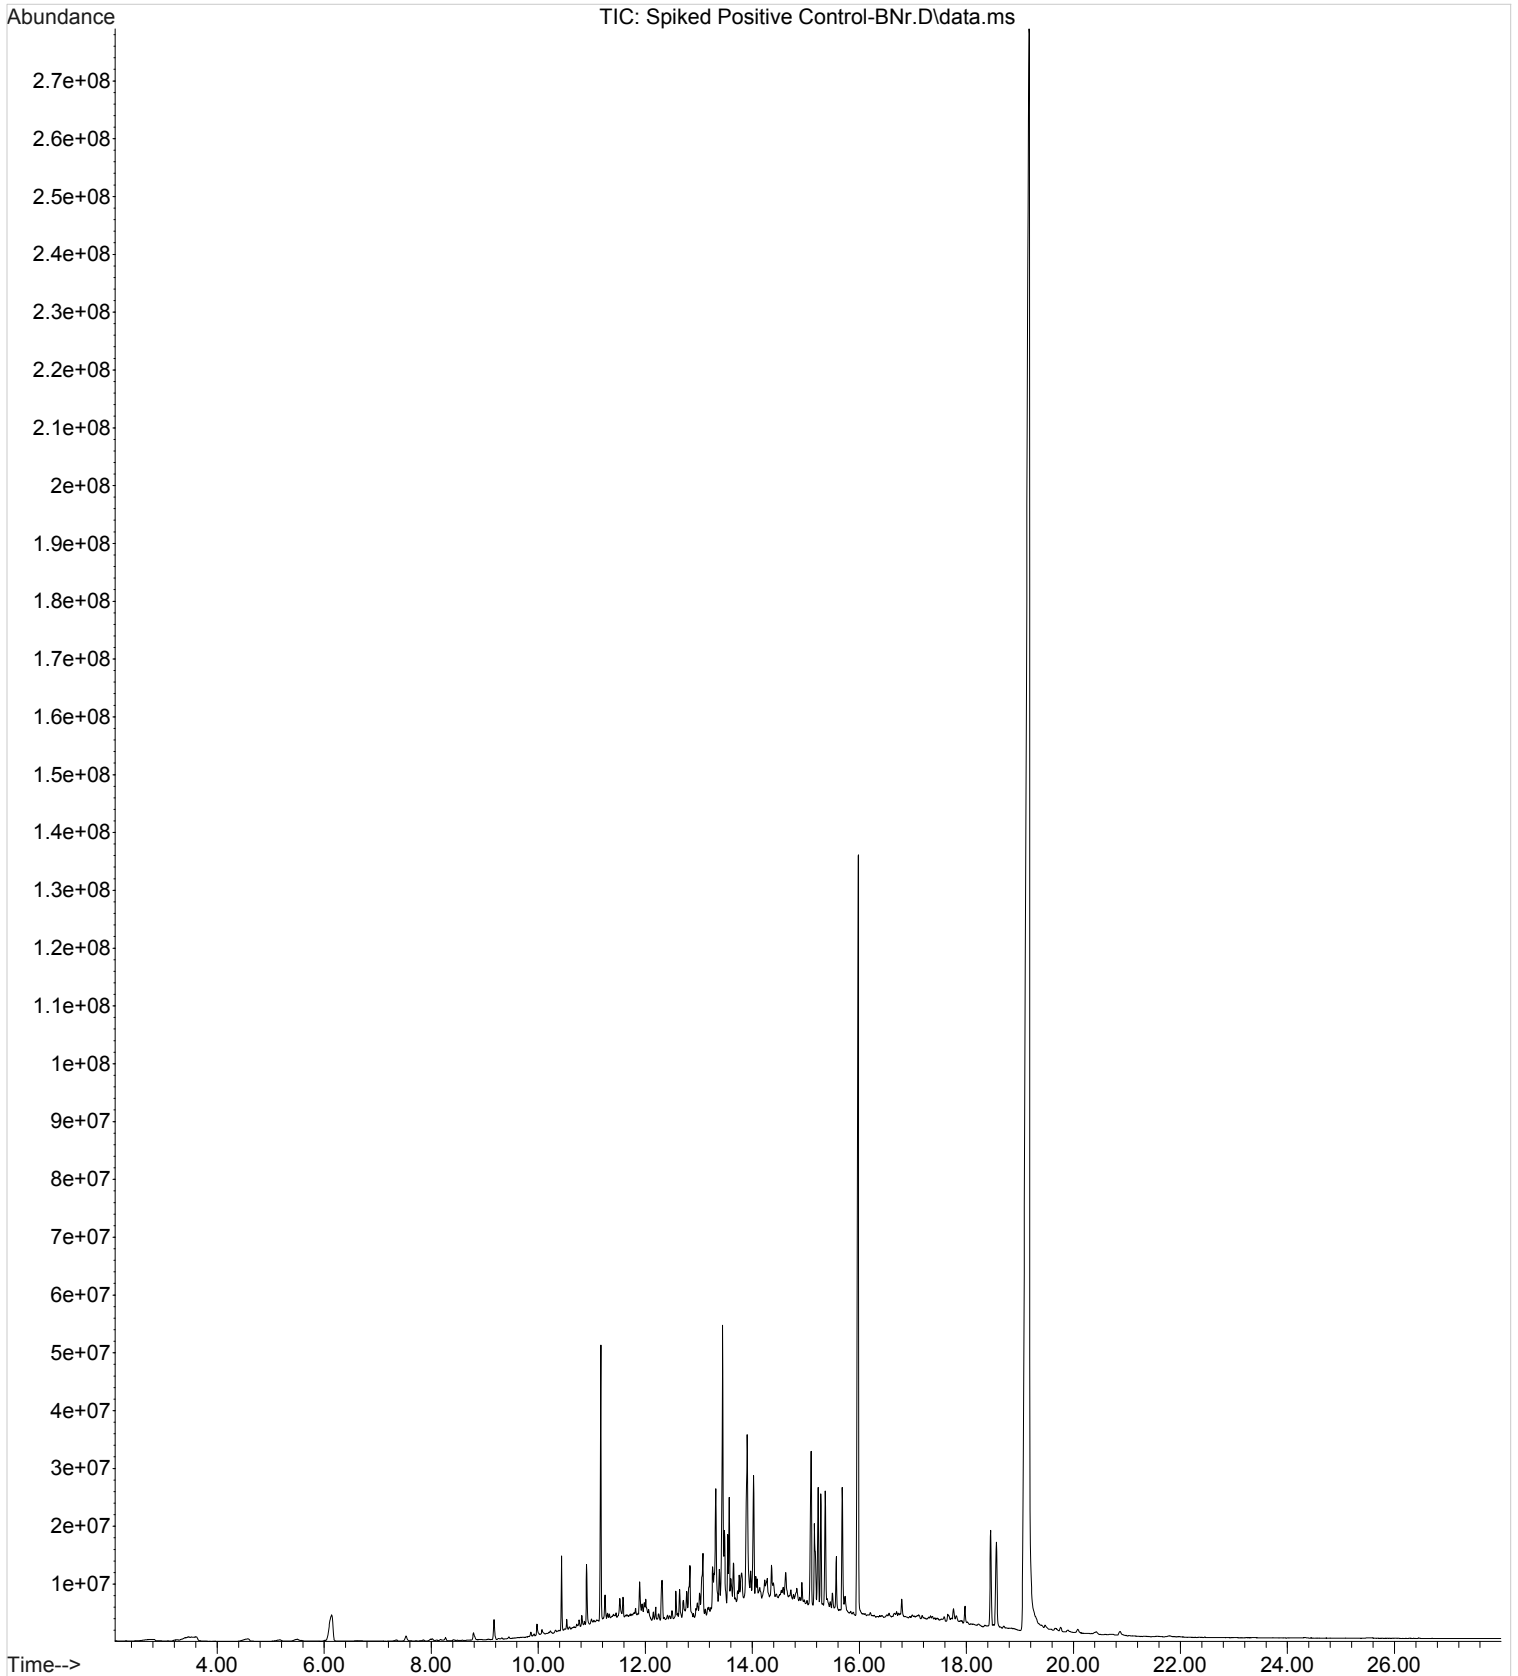



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2017\042817
... \Spiked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 28 Apr 2017 13:41 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111616

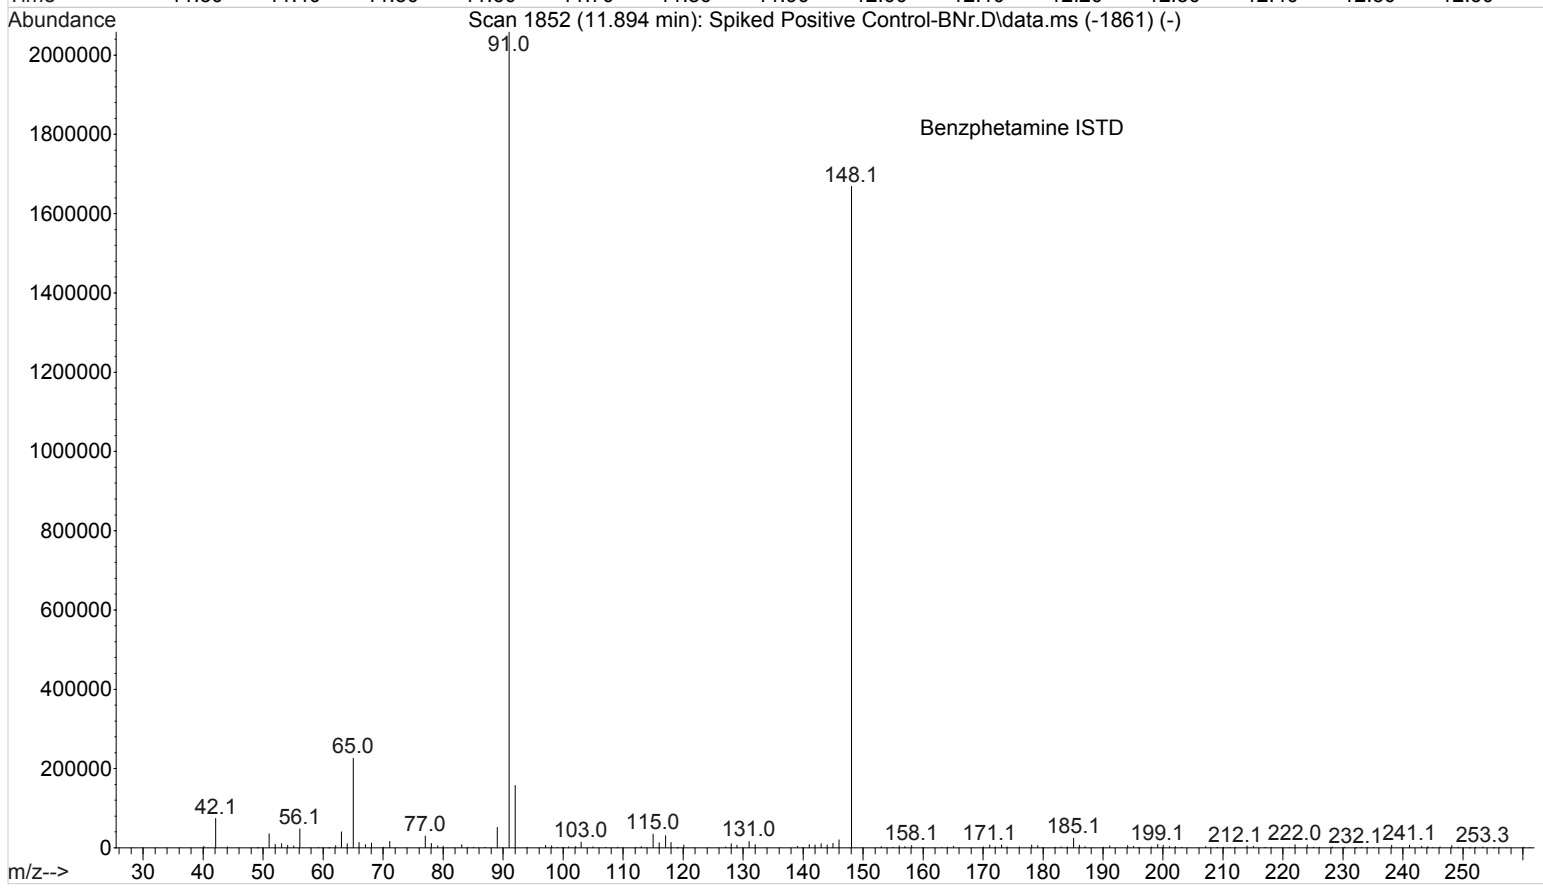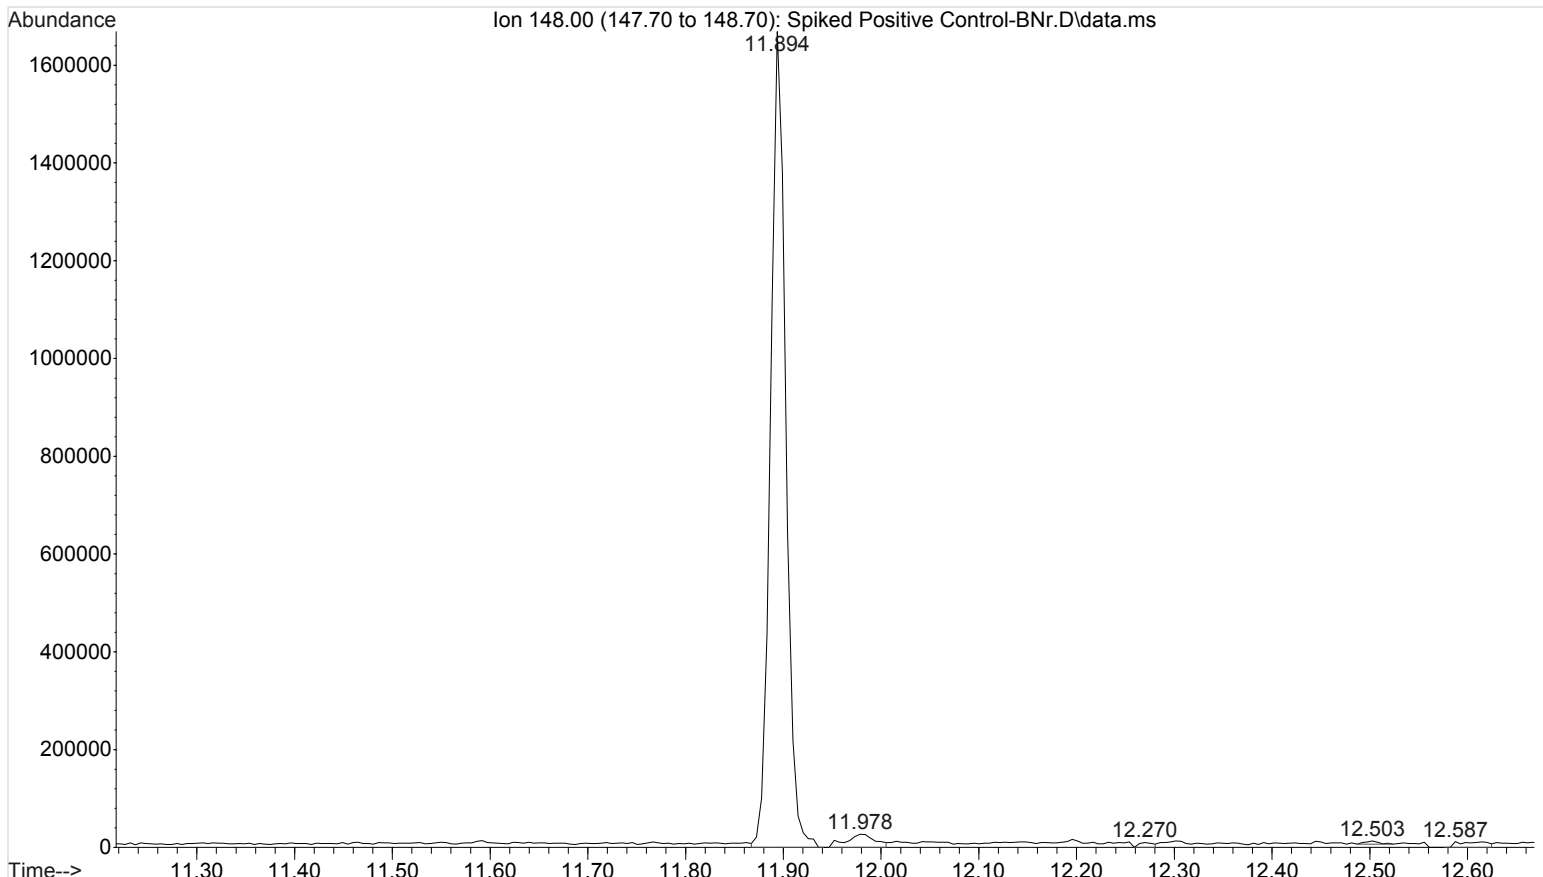



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2017\042817
... \Spiked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 28 Apr 2017 13:41 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111616

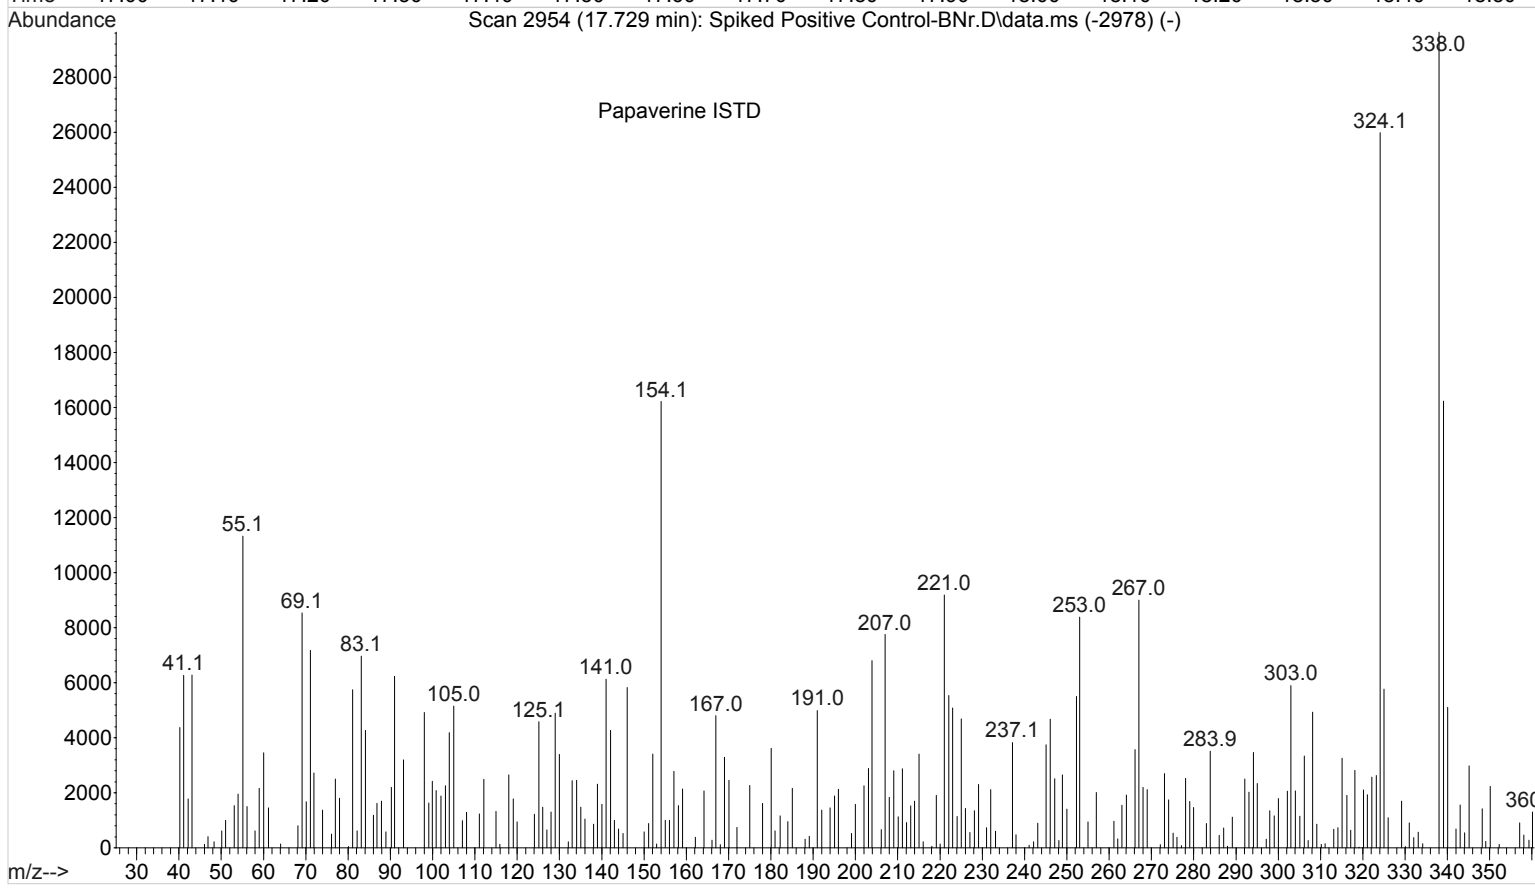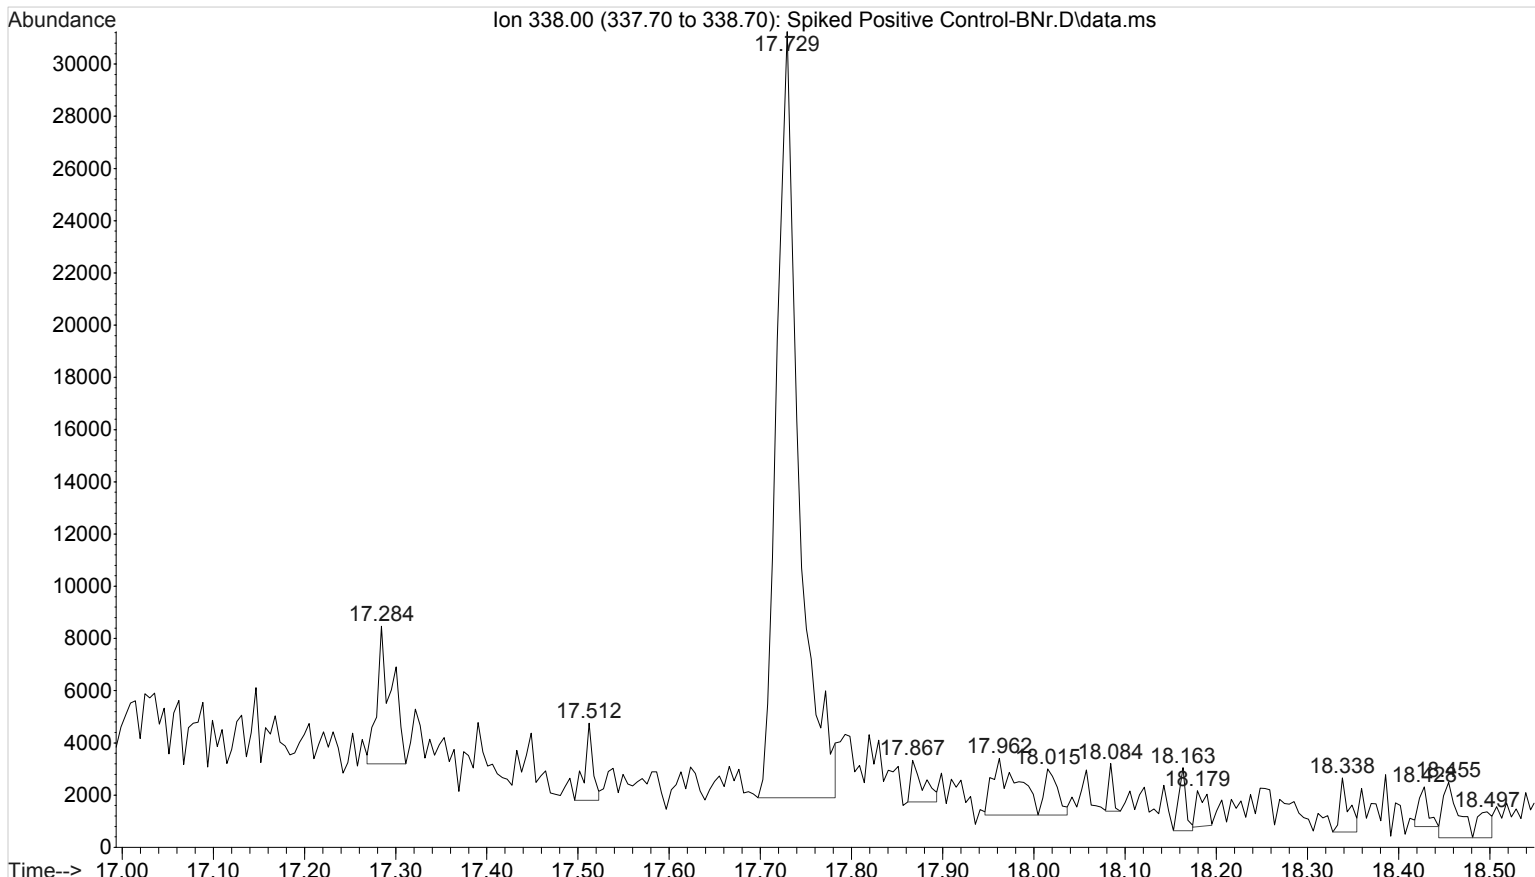

File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2017\042817
... \Spiked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 28 Apr 2017 13:41 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111616

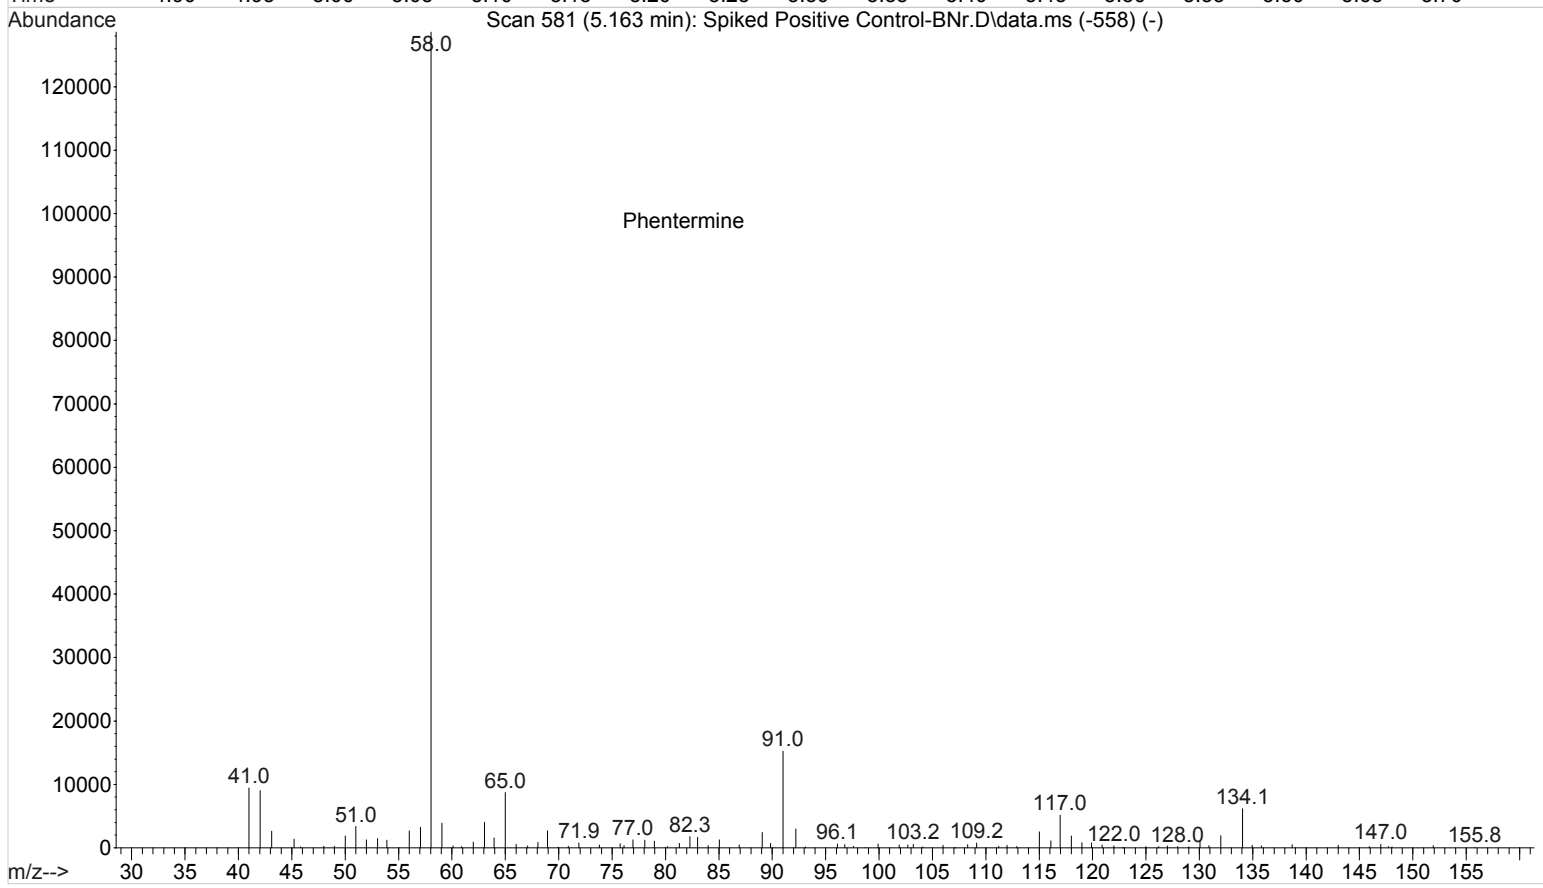
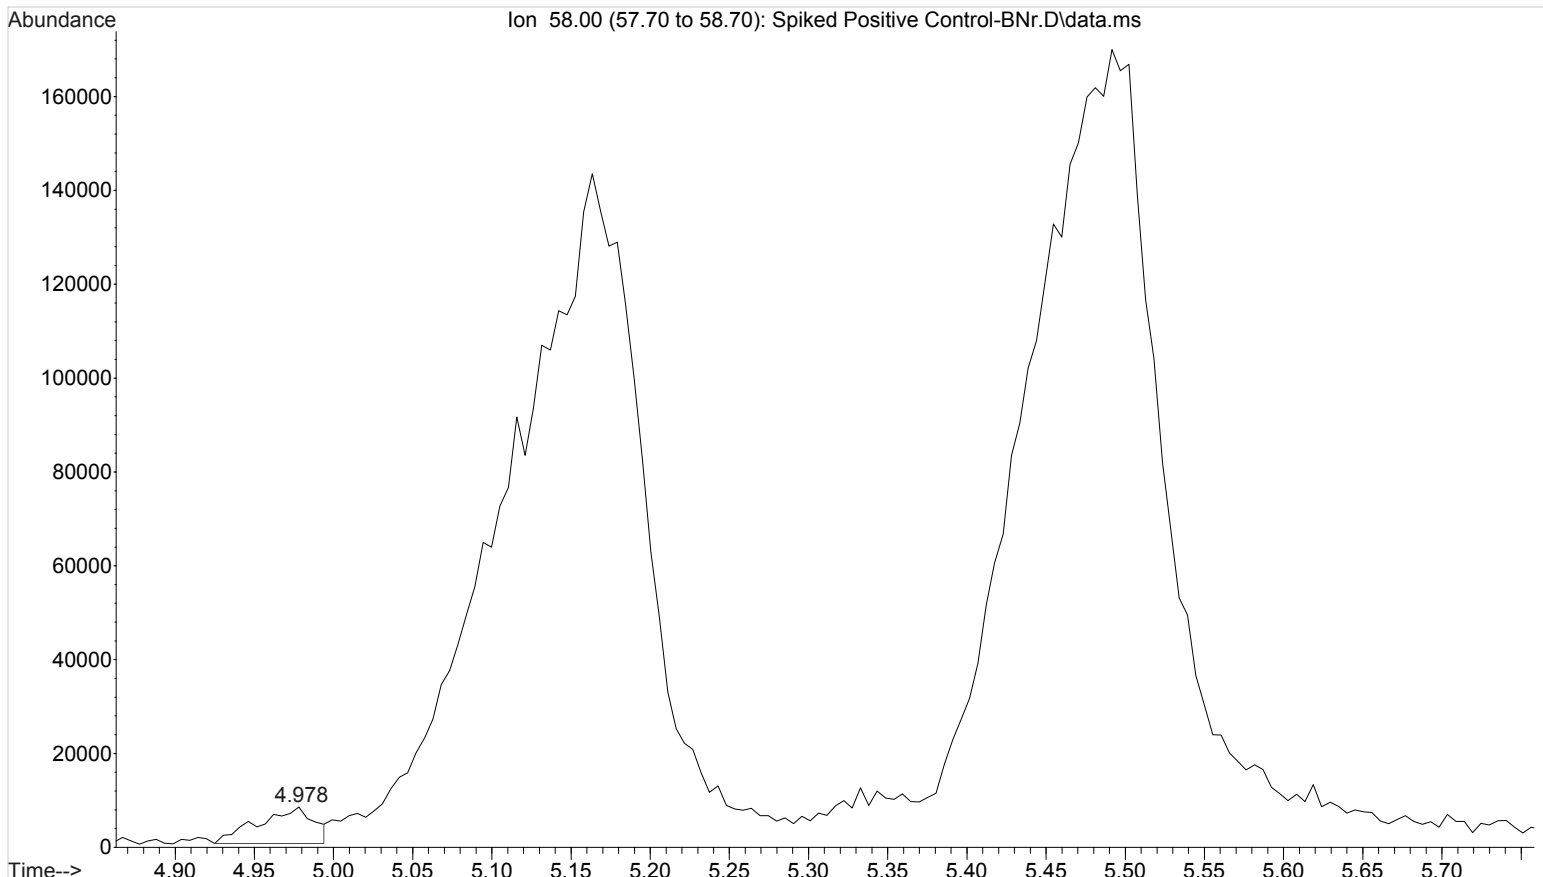


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2017\042817
... \Spiked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 28 Apr 2017 13:41 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111616

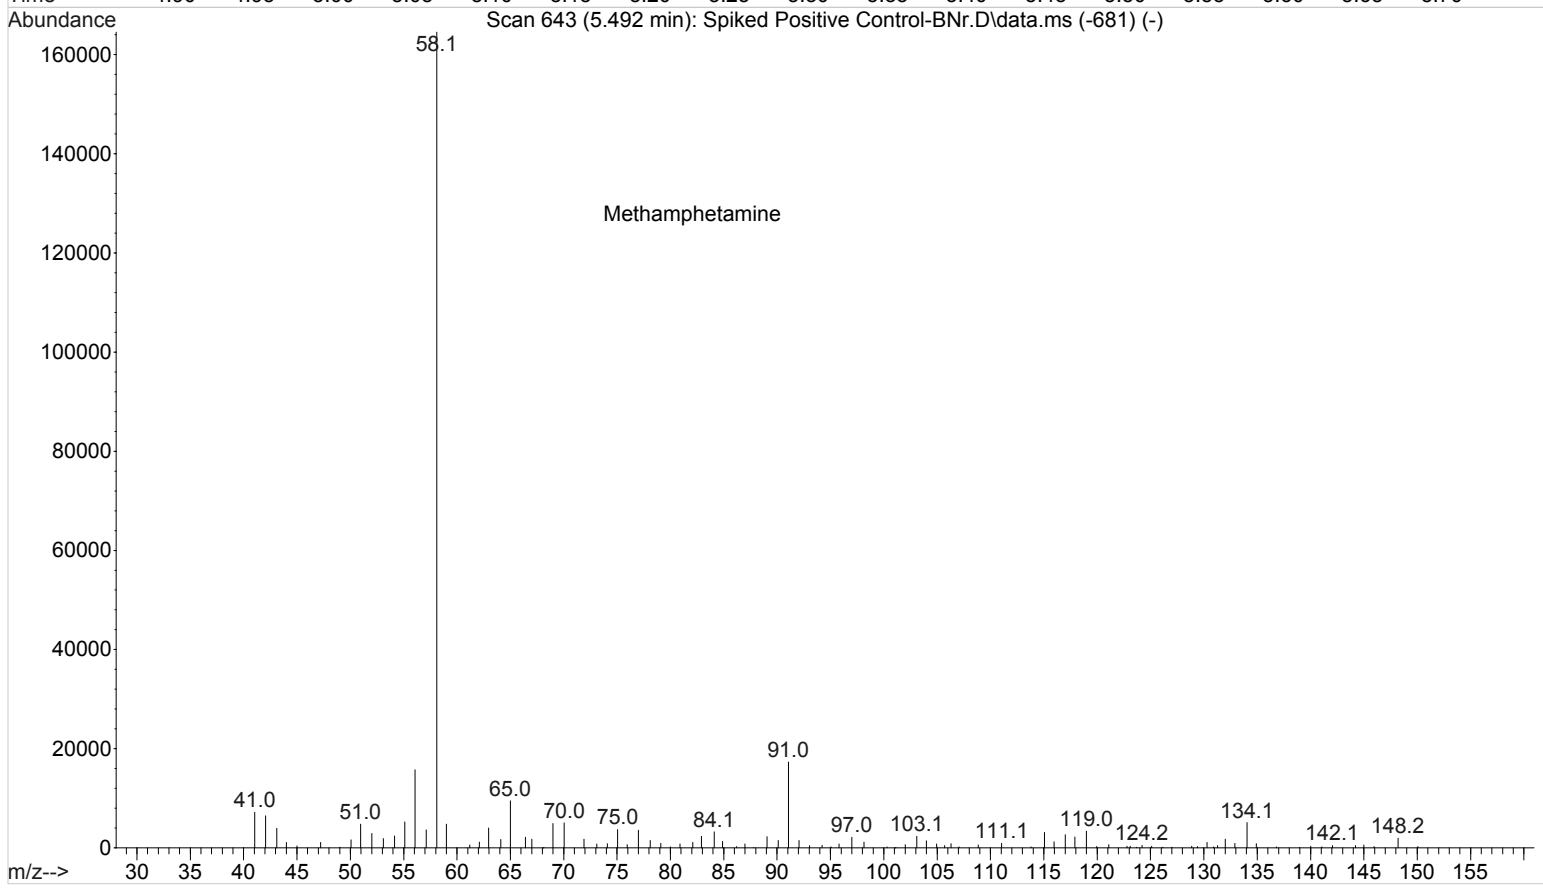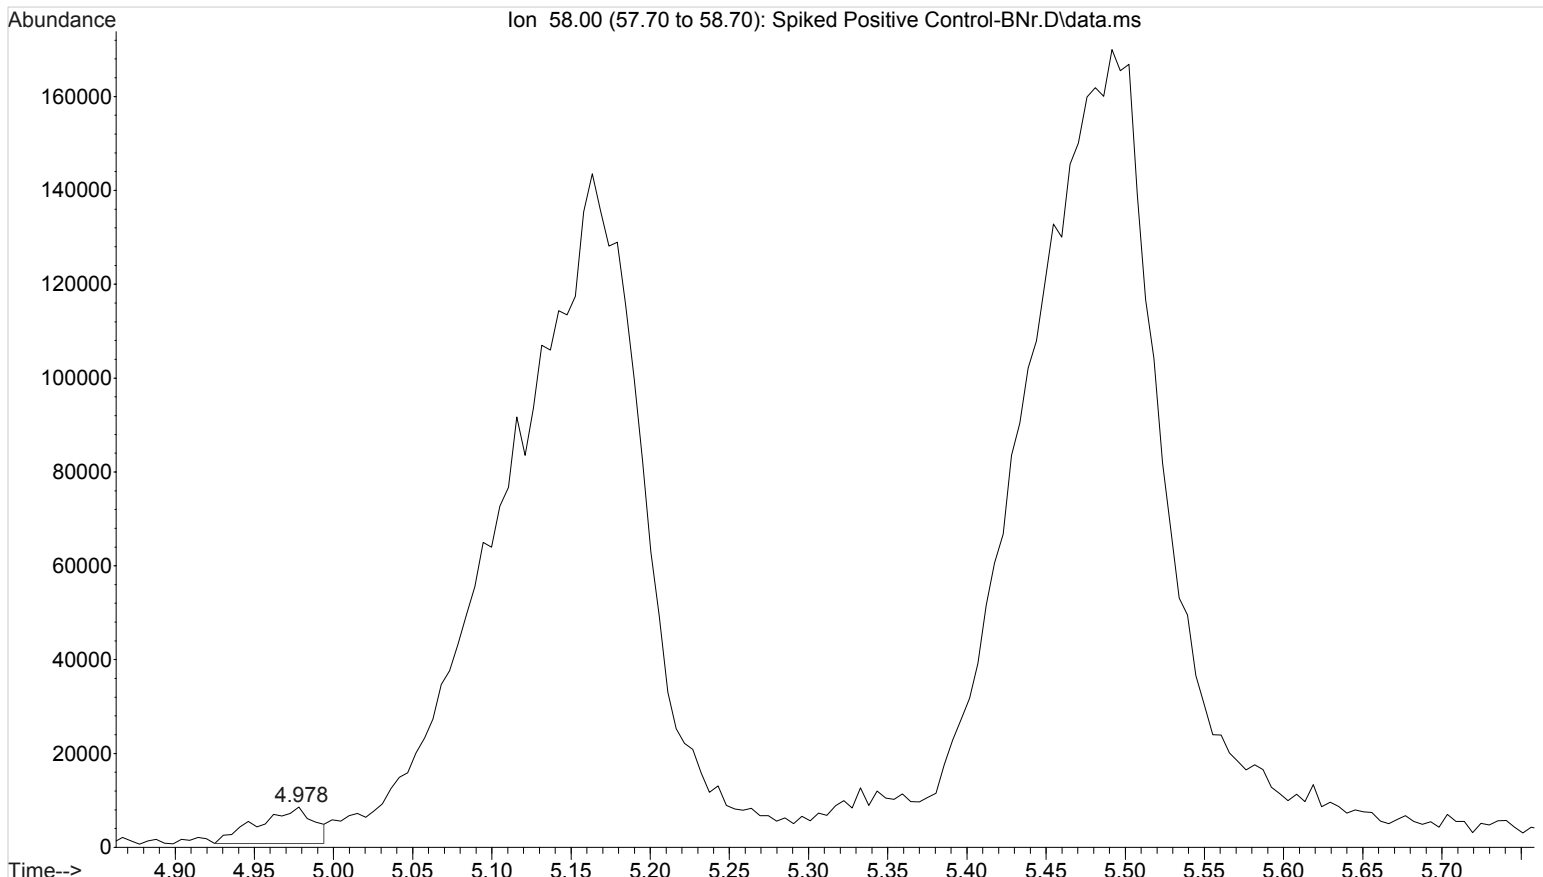



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2017\042817
... \Spiked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 28 Apr 2017 13:41 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111616

CS

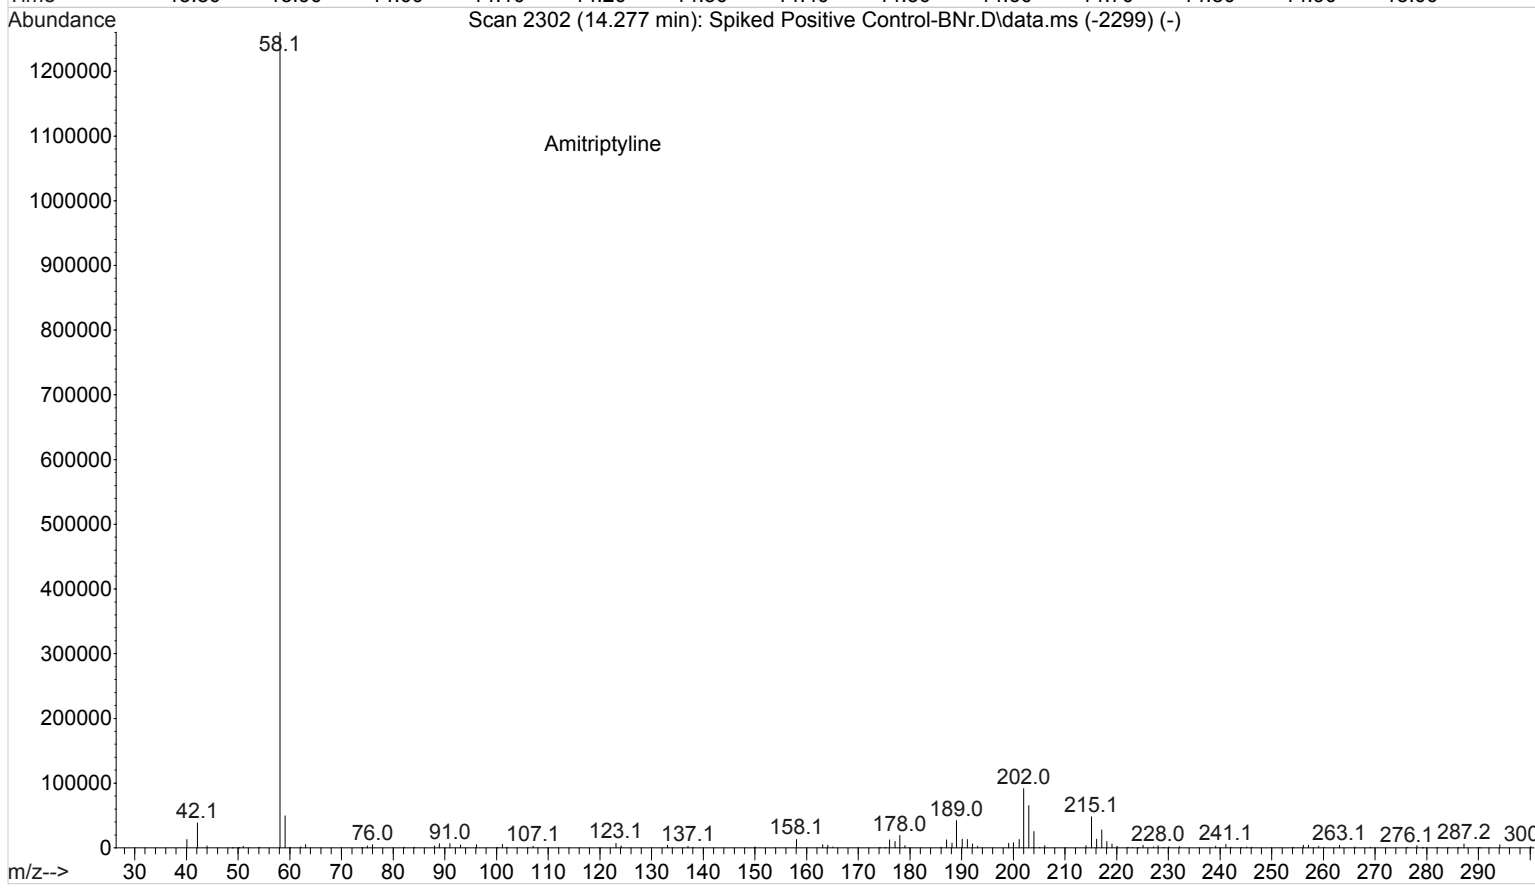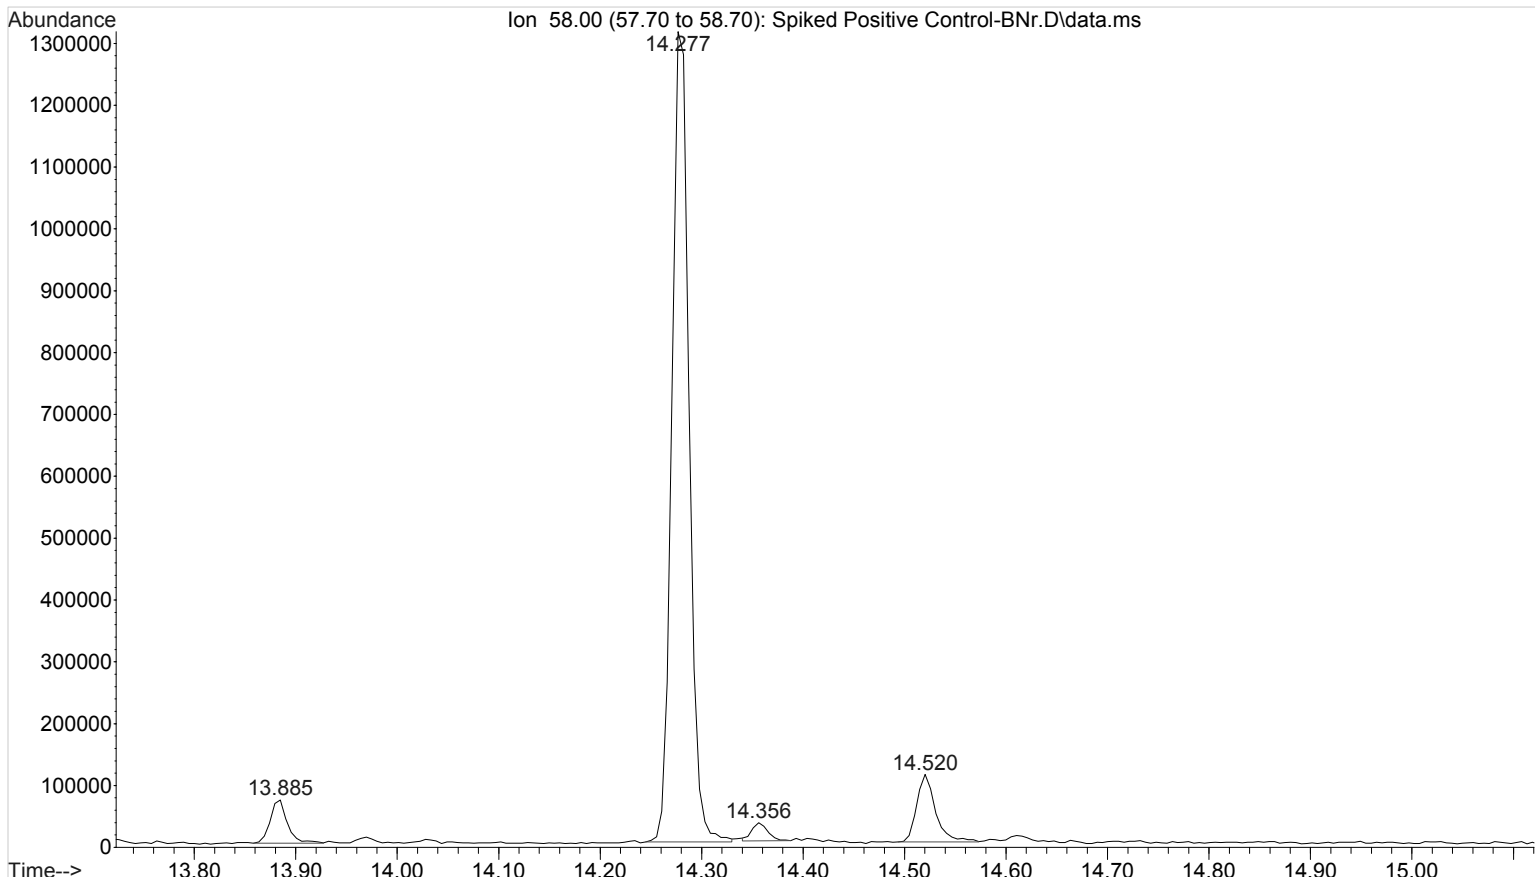

File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2017\042817
... \Spiked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 28 Apr 2017 13:41 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111616

6

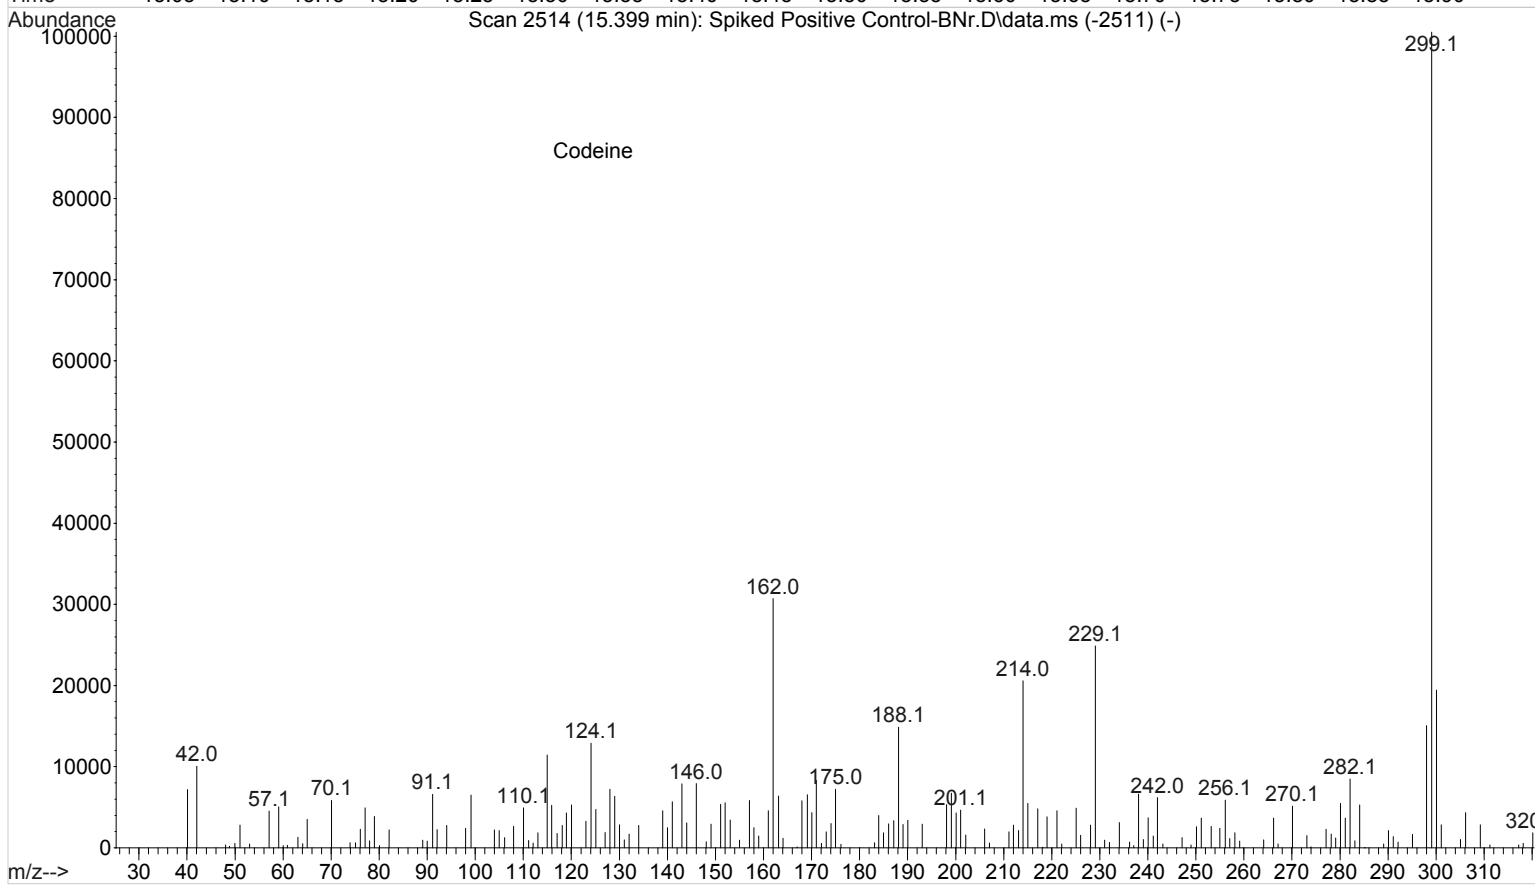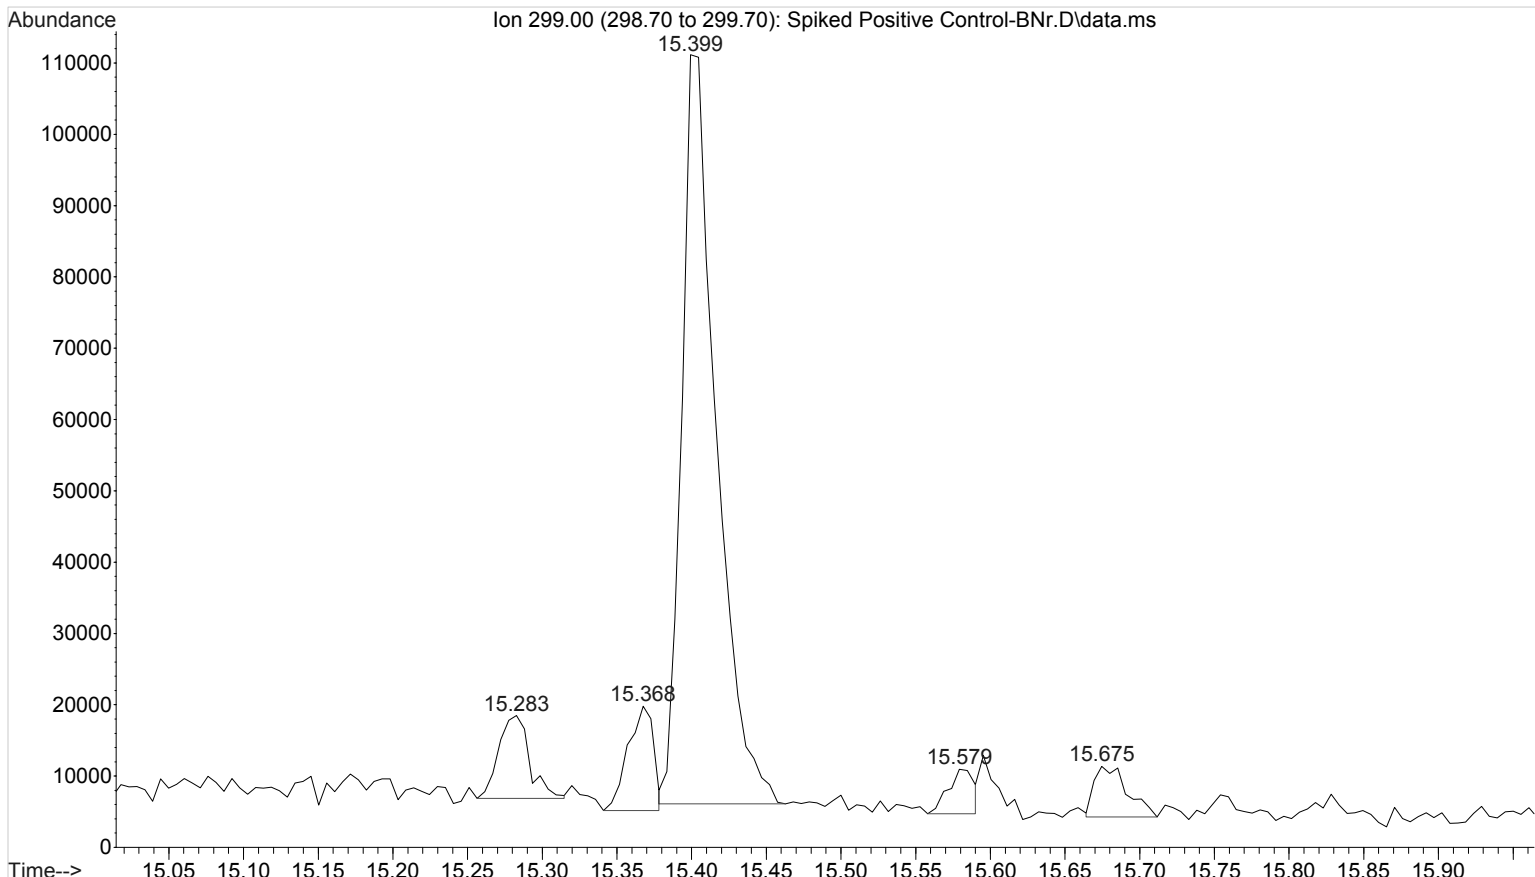

File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2017\042817
... \Spiked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 28 Apr 2017 13:41 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111616

