
























Worklist: 1201

<u>LAB_CASE</u>	<u>ITEM</u>	<u>TASK_ID</u>	<u>DESCRIPTION</u>	
C2016-0225	1	50442	3.6.1 Blood base neutral confirr	
M2016-0433	3	50454	3.6.1 Blood base neutral confirr	
M2016-0481	1	50253	3.6.1 Blood base neutral confirr	
M2016-0521	1	50433	3.6.1 Blood base neutral confirr	
M2016-0531	1	50487	3.6.1 Blood base neutral confirr	
M2016-0594	2	50706	3.6.1 Blood base neutral confirr	
M2016-0608	1	50800	3.6.1 Blood base neutral confirr	
M2016-0615	1	50861	3.6.1 Blood base neutral confirr	
M2016-0674	1	51159	3.6.1 Blood base neutral confirr	
M2016-0707	1	51336	3.6.1 Blood base neutral confirr	
P2016-0264	1	50234	3.6.1 Blood base neutral confirr	
P2016-0265	1	50237	3.6.1 Blood base neutral confirr	
P2016-0297	4	50637	3.6.1 Blood base neutral confirr	
P2016-0321	1	50651	3.6.1 Blood base neutral confirr	
P2016-0357	1	51049	3.6.1 Blood base neutral confirr	
P2016-0386	1	51179	3.6.1 Blood base neutral confirr	
P2016-0405	1	51315	3.6.1 Blood base neutral confirr	
P2016-0419	1	51376	3.6.1 Blood base neutral confirr	
P2016-0420	1	51379	3.6.1 Blood base neutral confirr	
P2016-0421	1	51382	3.6.1 Blood base neutral confirr	
P2016-0422	1	51385	3.6.1 Blood base neutral confirr	
P2016-0436	1	51571	3.6.1 Blood base neutral confirr	
P2016-0519	1	52061	3.6.1 Blood base neutral confirr	

Worklist: 1201

<u>LAB CASE</u>	<u>ITEM</u>	<u>TASK ID</u>	<u>DESCRIPTION</u>
P2016-0526	1	52082	3.6.1 Blood base neutral confirr
P2016-1382	1	58298	3.6.1 Blood base neutral confirr



Reviewed 7/21/16

A handwritten signature in green ink, consisting of several overlapping loops and a long horizontal stroke extending to the right.

9

simulate_sequence.log
 Simulate Run Sequence Thu Jul 14 15:46:35 2016

Instrument Name: Major Mass Spec
 Sequence File: C:\Users\ISPuser\Desktop\Sequences\CS-BNSB061616.sequence.xml
 Comment: MassHunter sequence
 Operator: ISP\datastor
 Data Path: D:\DATA\CDS\2016\071416\
 Method Path: C:\Users\datastor\Desktop\OP Methods\

Line	Type	Vials	DataFile	Sample Name
Acquisition Method: BNSB120510.M				
1)	Sample	100	Prerun Solvent Blank	Pre-run Solvent Blank
2)	Sample	1	Negative Control-BN	Negative Control -
...	1013			
3)	Sample	2	Spiked Positive Control-BN	Positive Control
4)	Sample	99	prBLK2	Solvent Blank
Acquisition Method: GBT092509-Delta EMV.M				
5)	Sample	100	Prerun Solvent Blankr	Pre-run Solvent Blank
6)	Sample	1	Negative Control-BNr	Negative Control -
...	1013			
7)	Sample	2	Spiked Positive Control-BNr	Positive Control
8)	Sample	99	prBLK2r	Solvent Blank
Acquisition Method: BNSB120510.M				
9)	Sample	100	C2016-0225-1-BNBLK	Lab No.: C2016-0225-1
10)	Sample	3	C2016-0225-1-BN	Lab No.: C2016-0225-1
11)	Sample	100	M2016-0433-3-BNBLK	Lab No.: M2016-0433-3
12)	Sample	4	M2016-0433-3-BN	Lab No.: M2016-0433-3
13)	Sample	100	M2016-0481-1-BNBLK	Lab No.: M2016-0481-1
14)	Sample	5	M2016-0481-1-BN	Lab No.: M2016-0481-1
15)	Sample	100	M2016-0521-1-BNBLK	Lab No.: M2016-0521-1
16)	Sample	6	M2016-0521-1-BN	Lab No.: M2016-0521-1
17)	Sample	100	M2016-0531-1-BNBLK	Lab No.: M2016-0531-1
18)	Sample	7	M2016-0531-1-BN	Lab No.: M2016-0531-1
19)	Sample	100	M2016-0594-2-BNBLK	Lab No.: M2016-0594-2
20)	Sample	8	M2016-0594-2-BN	Lab No.: M2016-0594-2
21)	Sample	100	M2016-0608-1-BNBLK	Lab No.: M2016-0608-1
22)	Sample	9	M2016-0608-1-BN	Lab No.: M2016-0608-1
23)	Sample	100	M2016-0615-1-BNBLK	Lab No.: M2016-0615-1
24)	Sample	10	M2016-0615-1-BN	Lab No.: M2016-0615-1
Acquisition Method: GBT092509-Delta EMV.M				
25)	Sample	100	C2016-0225-1-BNBLKr	Lab No.: C2016-0225-1
26)	Sample	3	C2016-0225-1-BNr	Lab No.: C2016-0225-1
27)	Sample	100	M2016-0433-3-BNBLKr	Lab No.: M2016-0433-3
28)	Sample	4	M2016-0433-3-BNr	Lab No.: M2016-0433-3
29)	Sample	100	M2016-0481-1-BNBLKr	Lab No.: M2016-0481-1
30)	Sample	5	M2016-0481-1-BNr	Lab No.: M2016-0481-1
31)	Sample	100	M2016-0521-1-BNBLKr	Lab No.: M2016-0521-1
32)	Sample	6	M2016-0521-1-BNr	Lab No.: M2016-0521-1
33)	Sample	100	M2016-0531-1-BNBLKr	Lab No.: M2016-0531-1
34)	Sample	7	M2016-0531-1-BNr	Lab No.: M2016-0531-1
35)	Sample	100	M2016-0594-2-BNBLKr	Lab No.: M2016-0594-2
36)	Sample	8	M2016-0594-2-BNr	Lab No.: M2016-0594-2
37)	Sample	100	M2016-0608-1-BNBLKr	Lab No.: M2016-0608-1
38)	Sample	9	M2016-0608-1-BNr	Lab No.: M2016-0608-1
39)	Sample	100	M2016-0615-1-BNBLKr	Lab No.: M2016-0615-1
40)	Sample	10	M2016-0615-1-BNr	Lab No.: M2016-0615-1
Acquisition Method: BNSB120510.M				
41)	Sample	100	M2016-0674-1-BNBLK	Lab No.: M2016-0674-1
42)	Sample	11	M2016-0674-1-BN	Lab No.: M2016-0674-1
43)	Sample	100	M2016-0707-1-BNBLK	Lab No.: M2016-0707-1
44)	Sample	12	M2016-0707-1-BN	Lab No.: M2016-0707-1

```

simulate_sequence.log
45) Sample      100      P2016-0264-1-BNBLK      Lab No.: P2016-0264-1
46) Sample      13       P2016-0264-1-BN        Lab No.: P2016-0264-1
47) Sample     100       P2016-0265-1-BNBLK      Lab No.: P2016-0265-1
48) Sample      14       P2016-0265-1-BN        Lab No.: P2016-0265-1
49) Sample     100       P2016-0297-4-BNBLK      Lab No.: P2016-0297-4
50) Sample      15       P2016-0297-4-BN        Lab No.: P2016-0297-4

Acquisition Method: GBT092509-Delta EMV.M
51) Sample     100       M2016-0674-1-BNBLKr     Lab No.: M2016-0674-1
52) Sample      11       M2016-0674-1-BNr        Lab No.: M2016-0674-1
53) Sample     100       M2016-0707-1-BNBLKr     Lab No.: M2016-0707-1
54) Sample      12       M2016-0707-1-BNr        Lab No.: M2016-0707-1
55) Sample     100       P2016-0264-1-BNBLKr     Lab No.: P2016-0264-1
56) Sample      13       P2016-0264-1-BNr        Lab No.: P2016-0264-1
57) Sample     100       P2016-0265-1-BNBLKr     Lab No.: P2016-0265-1
58) Sample      14       P2016-0265-1-BNr        Lab No.: P2016-0265-1
59) Sample     100       P2016-0297-4-BNBLKr     Lab No.: P2016-0297-4
60) Sample      15       P2016-0297-4-BNr        Lab No.: P2016-0297-4

Acquisition Method: BNSB120510.M
61) Sample      99       P2016-0321-1-BNBLK      Lab No.: P2016-0321-1
62) Sample      16       P2016-0321-1-BN        Lab No.: P2016-0321-1
63) Sample      99       P2016-0357-1-BNBLK      Lab No.: P2016-0357-1
64) Sample      17       P2016-0357-1-BN        Lab No.: P2016-0357-1
65) Sample      99       P2016-0386-1-BNBLK      Lab No.: P2016-0386-1
66) Sample      18       P2016-0386-1-BN        Lab No.: P2016-0386-1
67) Sample      99       P2016-0405-1-BNBLK      Lab No.: P2016-0405-1
68) Sample      19       P2016-0405-1-BN        Lab No.: P2016-0405-1
69) Sample      99       P2016-0419-1-BNBLK      Lab No.: P2016-0419-1
70) Sample      20       P2016-0419-1-BN        Lab No.: P2016-0419-1

Acquisition Method: GBT092509-Delta EMV.M
71) Sample      99       P2016-0321-1-BNBLKr     Lab No.: P2016-0321-1
72) Sample      16       P2016-0321-1-BNr        Lab No.: P2016-0321-1
73) Sample      99       P2016-0357-1-BNBLKr     Lab No.: P2016-0357-1
74) Sample      17       P2016-0357-1-BNr        Lab No.: P2016-0357-1
75) Sample      99       P2016-0386-1-BNBLKr     Lab No.: P2016-0386-1
76) Sample      18       P2016-0386-1-BNr        Lab No.: P2016-0386-1
77) Sample      99       P2016-0405-1-BNBLKr     Lab No.: P2016-0405-1
78) Sample      19       P2016-0405-1-BNr        Lab No.: P2016-0405-1
79) Sample      99       P2016-0419-1-BNBLKr     Lab No.: P2016-0419-1
80) Sample      20       P2016-0419-1-BNr        Lab No.: P2016-0419-1

Acquisition Method: BNSB120510.M
81) Sample      99       P2016-0420-1-BNBLK      Lab No.: P2016-0420-1
82) Sample      21       P2016-0420-1-BN        Lab No.: P2016-0420-1
83) Sample      99       P2016-0421-1-BNBLK      Lab No.: P2016-0421-1
84) Sample      22       P2016-0421-1-BN        Lab No.: P2016-0421-1
85) Sample      99       P2016-0422-1-BNBLK      Lab No.: P2016-0422-1
86) Sample      23       P2016-0422-1-BN        Lab No.: P2016-0422-1
87) Sample      99       P2016-0436-1-BNBLK      Lab No.: P2016-0436-1
88) Sample      24       P2016-0436-1-BN        Lab No.: P2016-0436-1
89) Sample      99       P2016-0519-1-BNBLK      Lab No.: P2016-0519-1
90) Sample      25       P2016-0519-1-BN        Lab No.: P2016-0519-1

Acquisition Method: GBT092509-Delta EMV.M
91) Sample      99       P2016-0420-1-BNBLKr     Lab No.: P2016-0420-1
92) Sample      21       P2016-0420-1-BNr        Lab No.: P2016-0420-1
93) Sample      99       P2016-0421-1-BNBLKr     Lab No.: P2016-0421-1
94) Sample      22       P2016-0421-1-BNr        Lab No.: P2016-0421-1
95) Sample      99       P2016-0422-1-BNBLKr     Lab No.: P2016-0422-1
96) Sample      23       P2016-0422-1-BNr        Lab No.: P2016-0422-1
97) Sample      99       P2016-0436-1-BNBLKr     Lab No.: P2016-0436-1
98) Sample      24       P2016-0436-1-BNr        Lab No.: P2016-0436-1
99) Sample      99       P2016-0519-1-BNBLKr     Lab No.: P2016-0519-1
100) Sample     25       P2016-0519-1-BNr        Lab No.: P2016-0519-1

Acquisition Method: BNSB120510.M

```

```

simulate_sequence.log
101) Sample          99      P2016-0526-1-BNBLK      Lab No.: P2016-0526-1
102) Sample          26      P2016-0526-1-BN        Lab No.: P2016-0526-1

Acquisition Method: GBT092509-Delta EMV.M
103) Sample          99      P2016-0526-1-BNBLKr    Lab No.: P2016-0526-1
104) Sample          26      P2016-0526-1-BNr       Lab No.: P2016-0526-1

Acquisition Method: BNSB120510.M
105) Sample          99      P2016-1382-1-BNBLK     Lab No.: P2016-1382-1
106) Sample          27      P2016-1382-1-BN        Lab No.: P2016-1382-1

Acquisition Method: GBT092509-Delta EMV.M
107) Sample          99      P2016-1382-1-BNBLKr    Lab No.: P2016-1382-1
108) Sample          27      P2016-1382-1-BNr       Lab No.: P2016-1382-1

Acquisition Method: BNSB120510.M
109) Sample          99      POSTBLK                 BLK

Acquisition Method: GBT092509-Delta EMV.M
110) Sample          99      AFTER                   BLK
megabytes Needed: 2820  Space on drive D: 234094
Sequence Verification Done!

```

Analytical Method 3.6.1 & 3.6.7 QA Check List

Run Start Date: 07/14/2016

Analyst: CS

(Short GC/MS temperature program)

Positive Control Compound List


- Phentermine
- Methamphetamine
- Nicotine
- Meperidine
- Caffeine
- Diphenhydramine
- Lidocaine
- PCP
- Methadone
- Amitriptyline
- Codeine
- Trazodone

Internal Standards


- Benzphetamine
- Papaverine

Optional back extraction **not** performed.
Reconstituted in MeOH.


File :I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Prerun Solvent Blank.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 15:54 using AcqMethod BNSB120510.M
Sample Name: Pre-run Solvent Blank
Misc Info : Chloroform

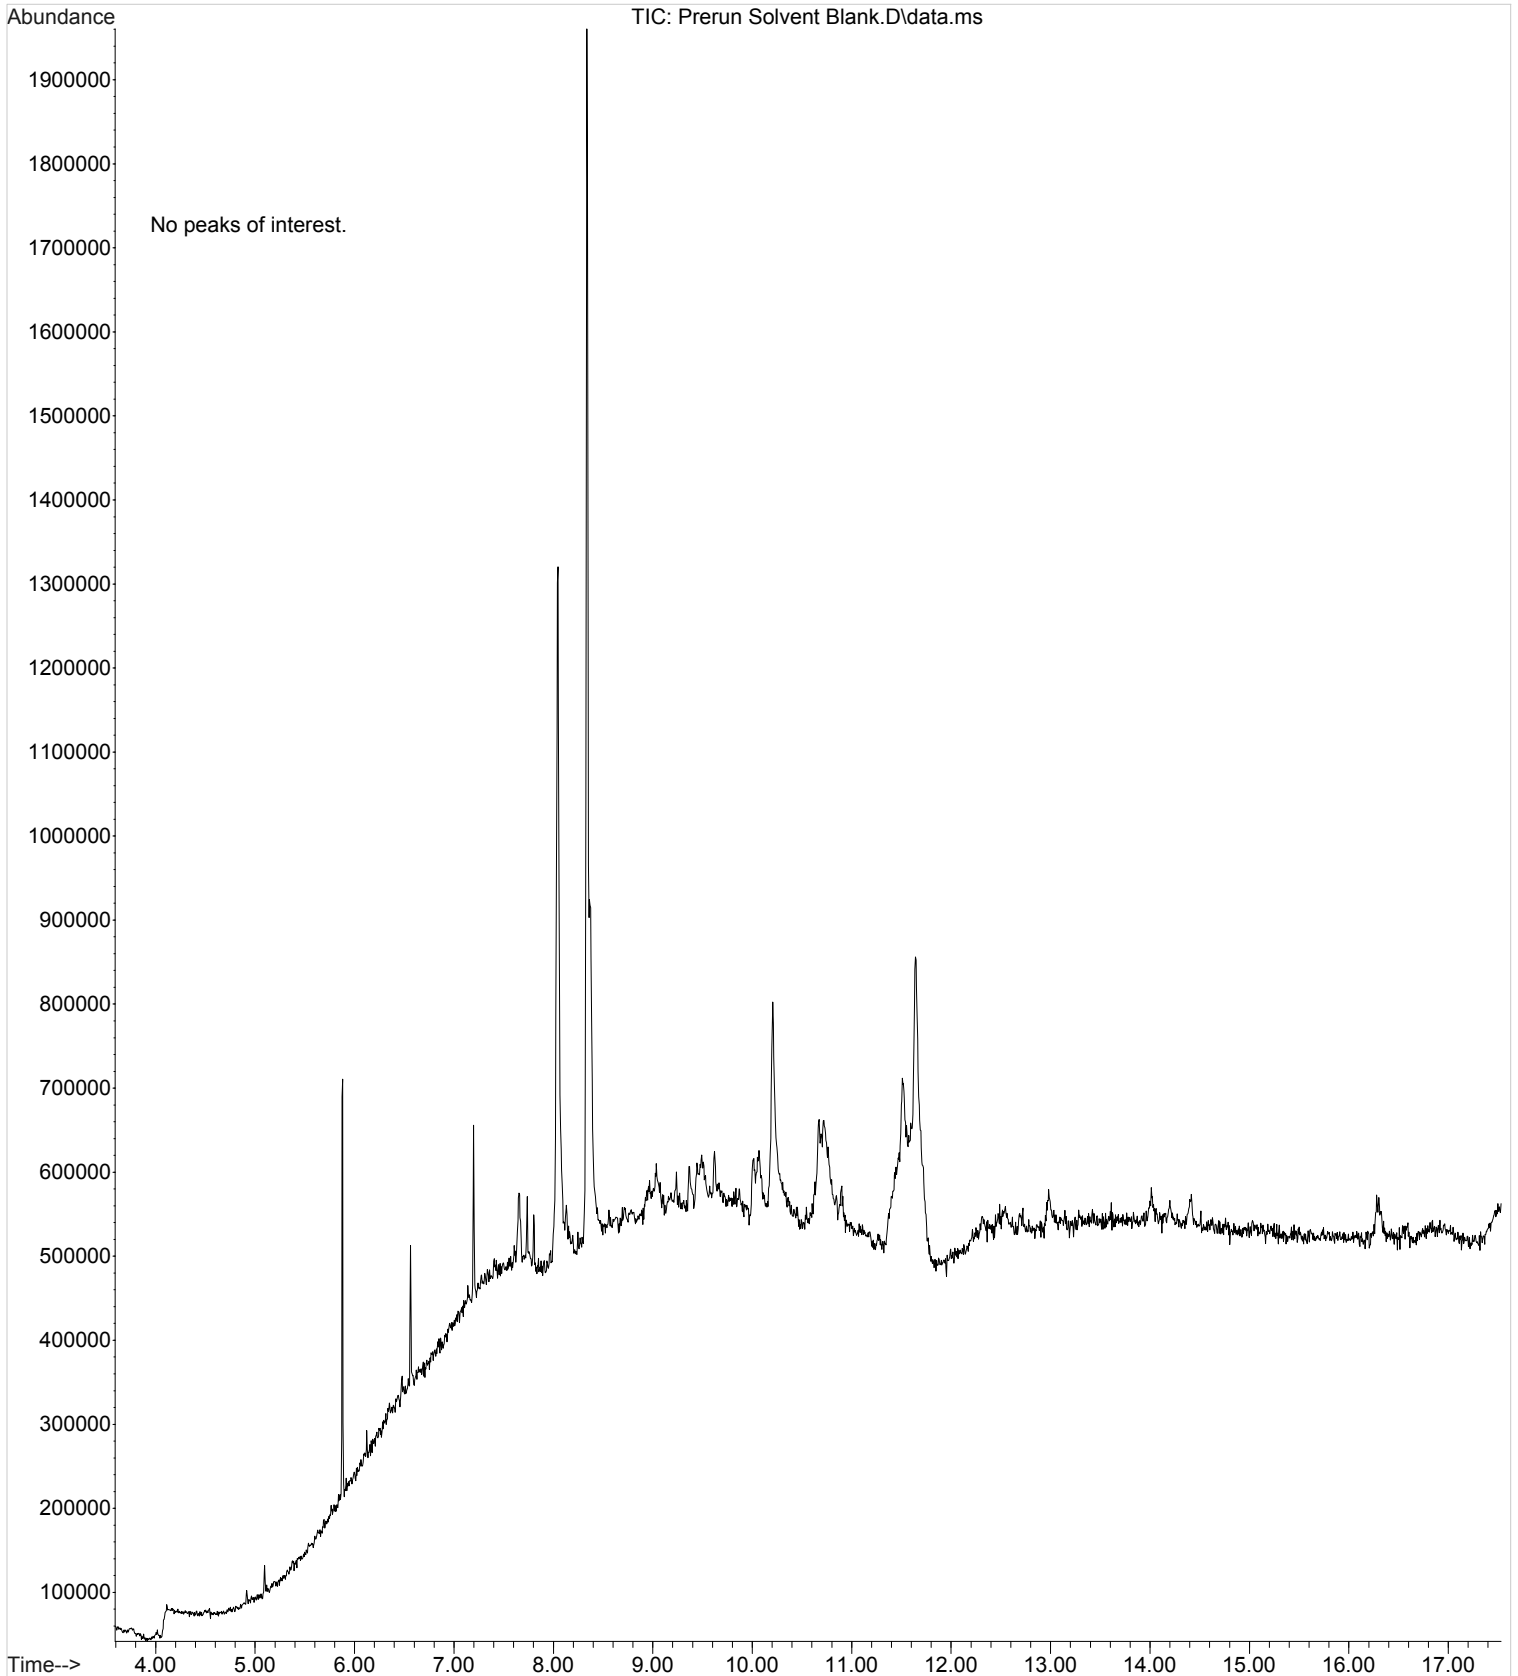

File :I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \prbLK2.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 17:03 using AcqMethod BNSB120510.M
Sample Name: Solvent Blank
Misc Info : Chloroform


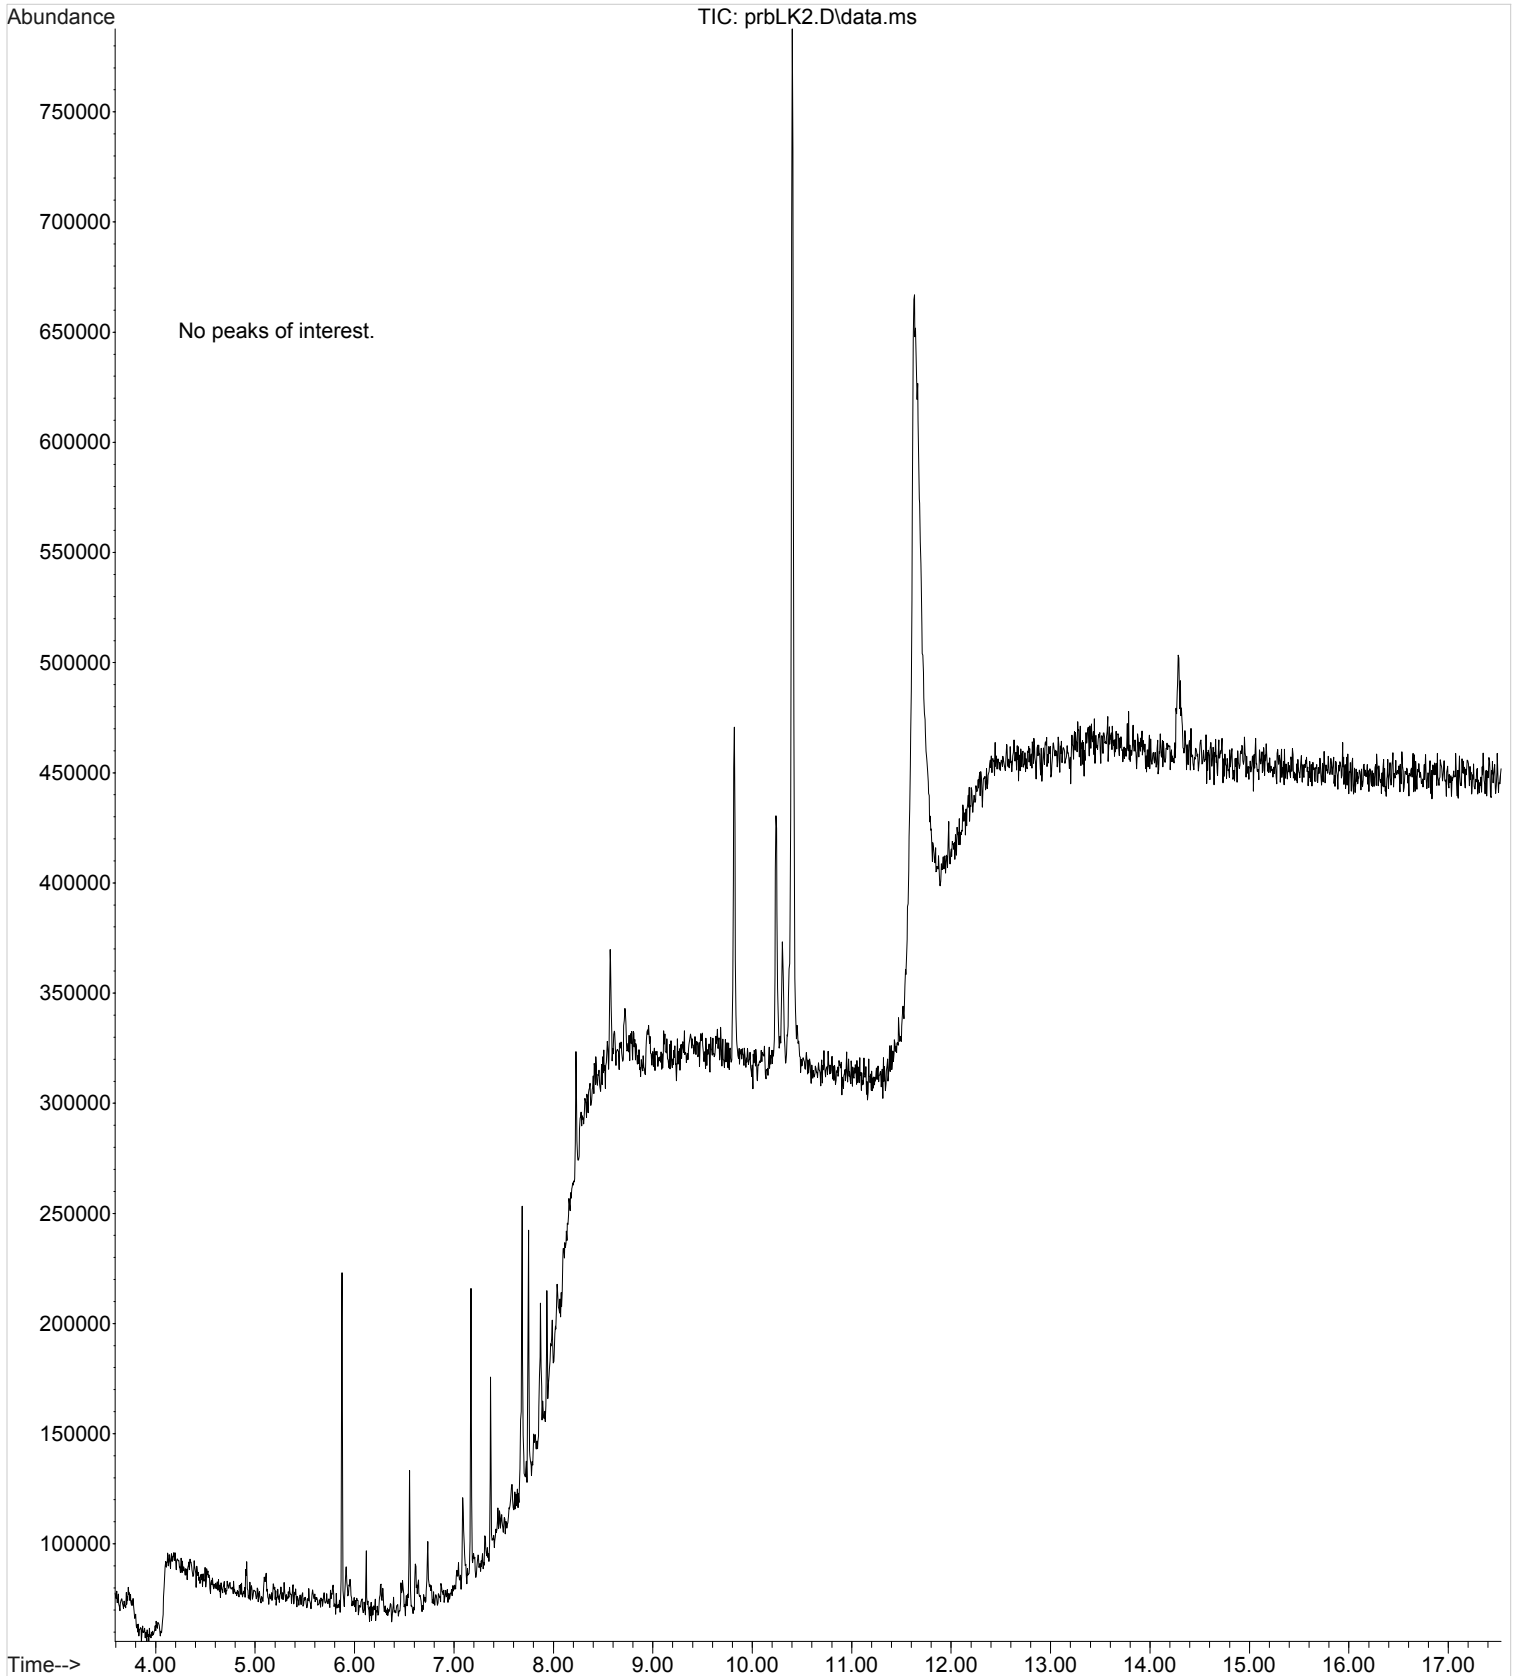


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Negative Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 17:59 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Negative Control - Utak Lot B1013
Misc Info : Analytical Method 3.6.1


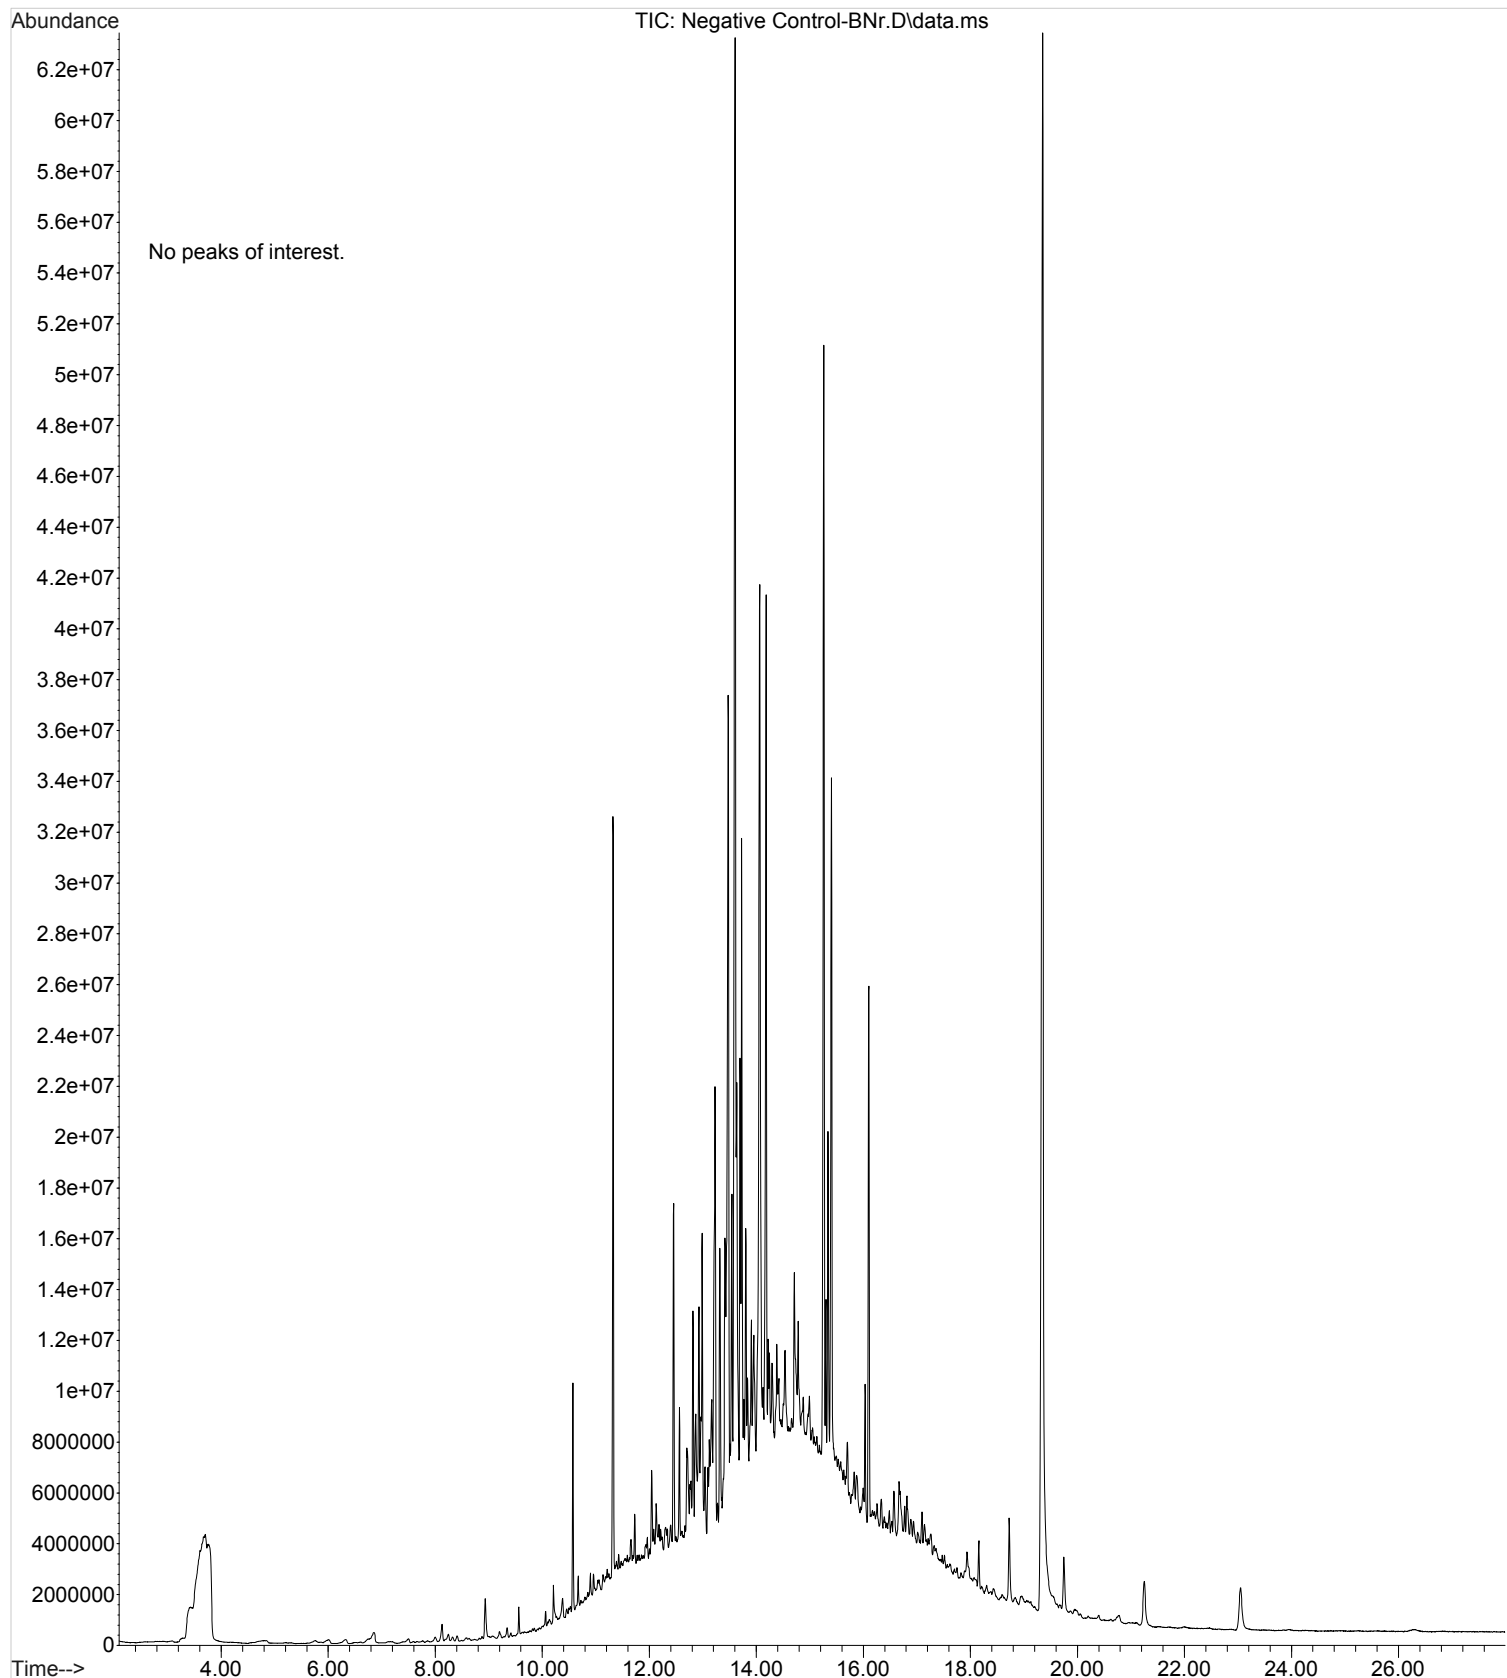


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Negative Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 16:17 using AcqMethod BNSB120510.M
Sample Name: Negative Control - Utak Lot B1013
Misc Info : Analytical Method 3.6.1

99

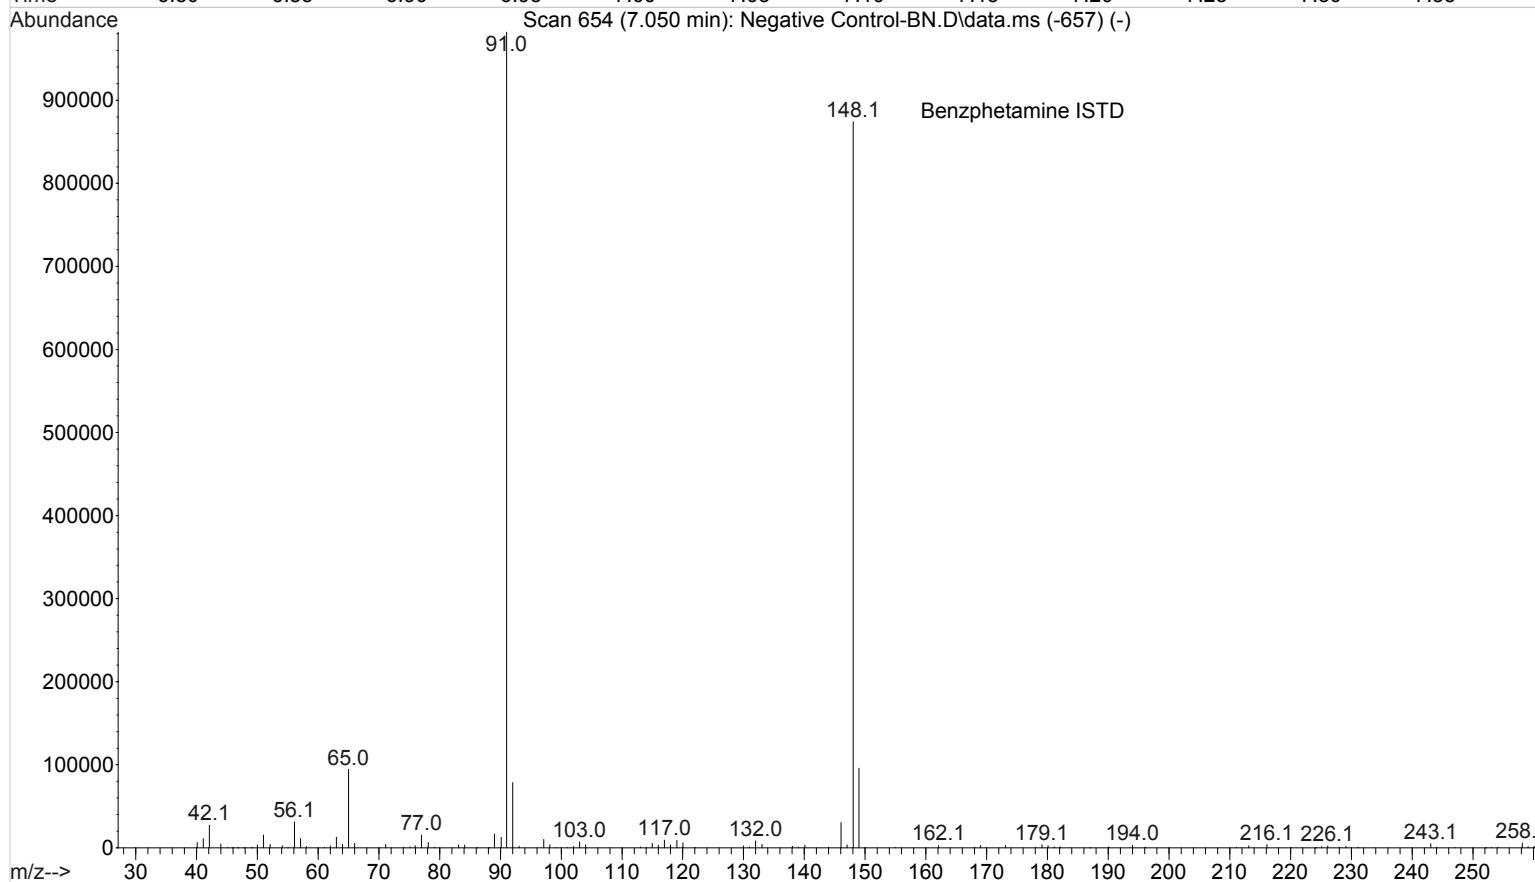
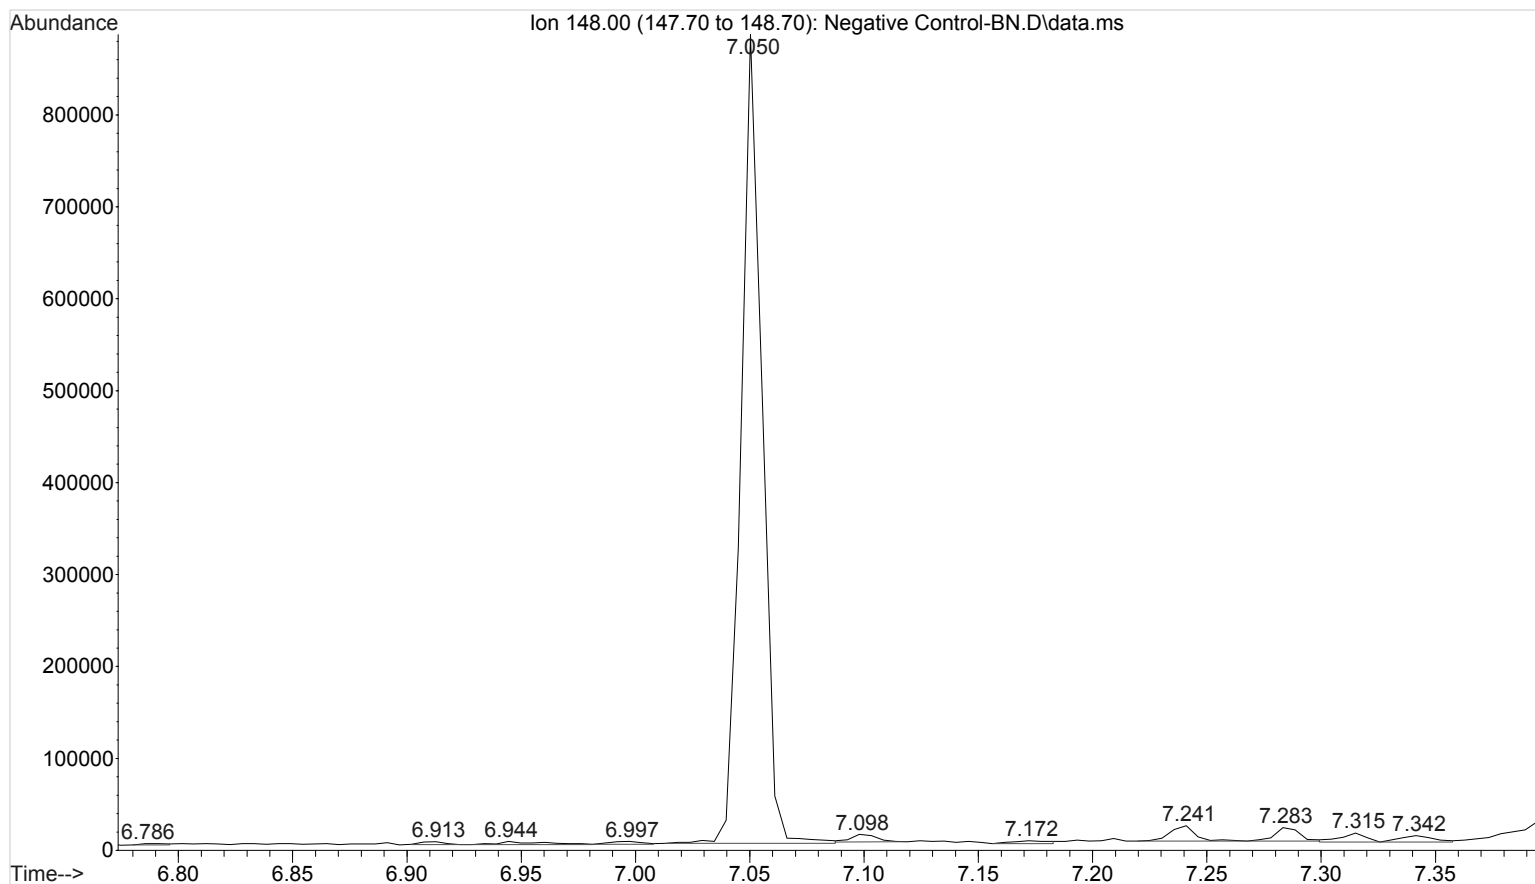


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Negative Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 16:17 using AcqMethod BNSB120510.M
Sample Name: Negative Control - Utak Lot B1013
Misc Info : Analytical Method 3.6.1

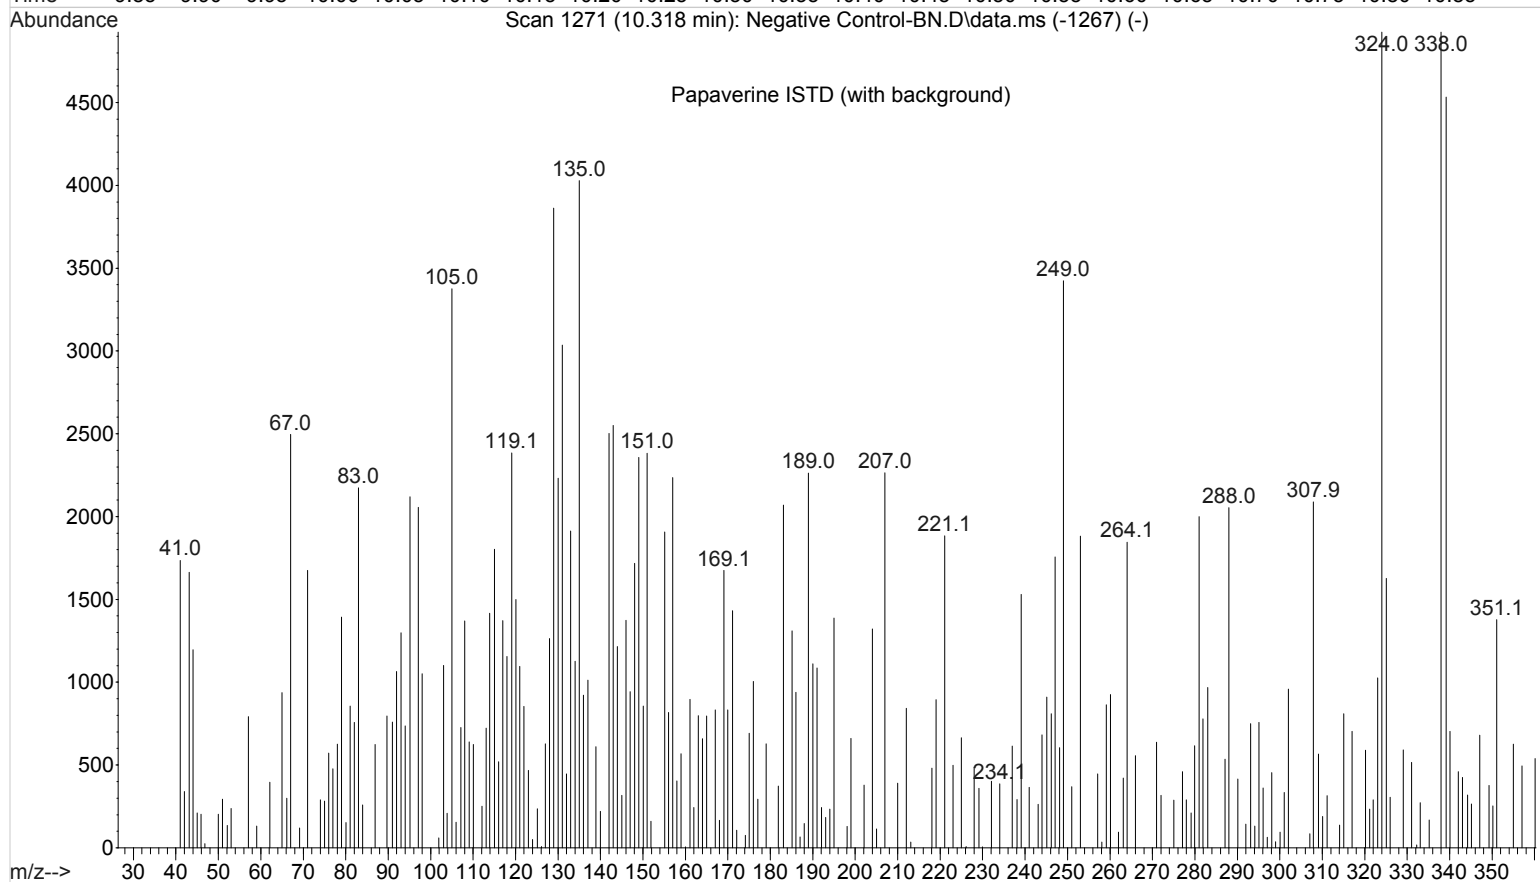
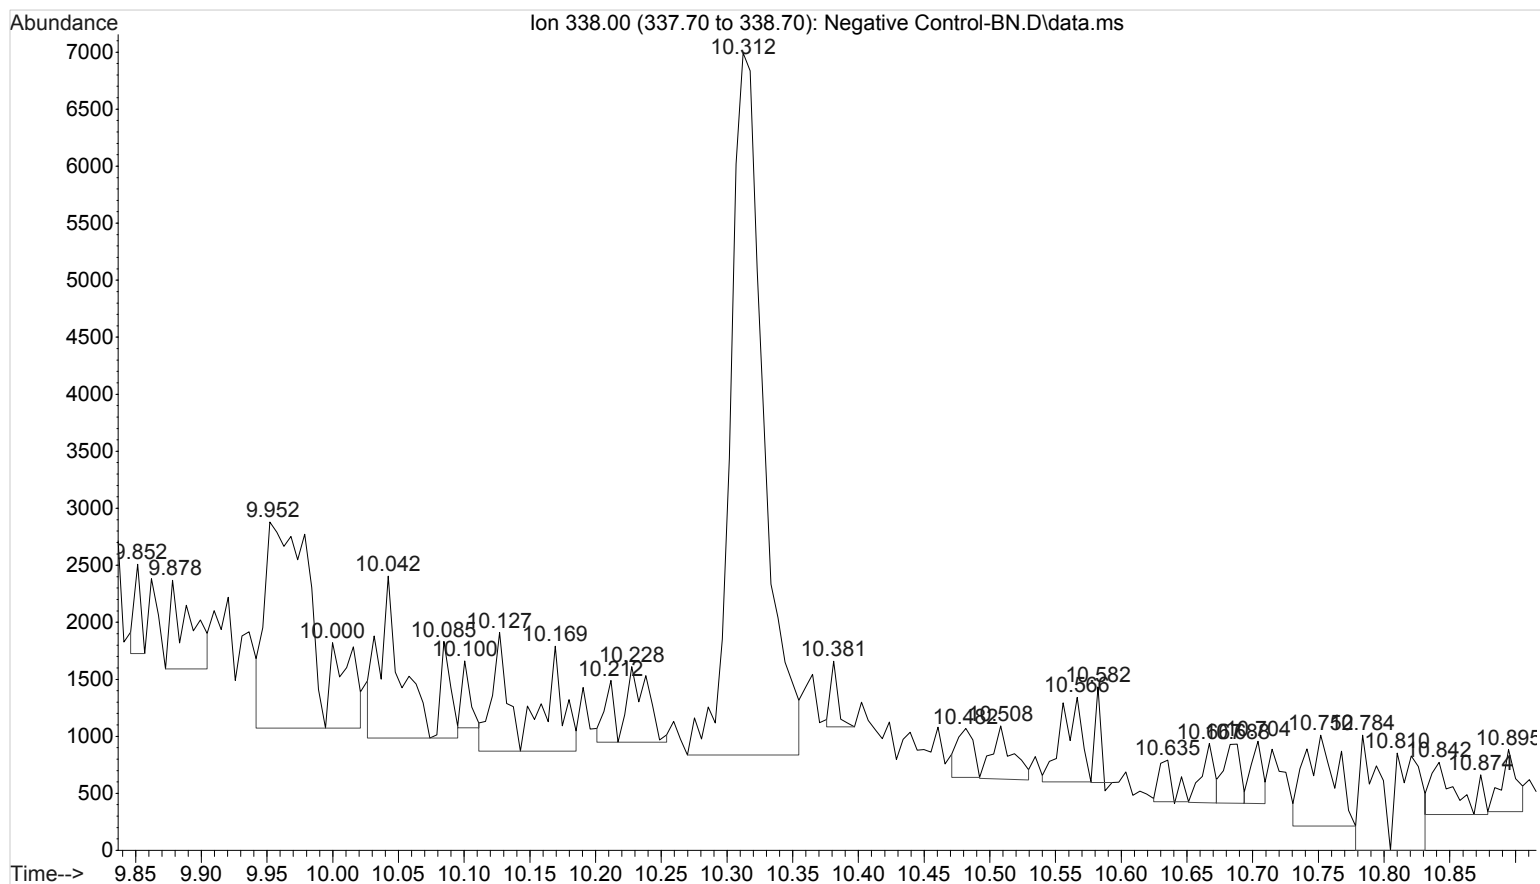


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Spiked Positive Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 16:40 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

9

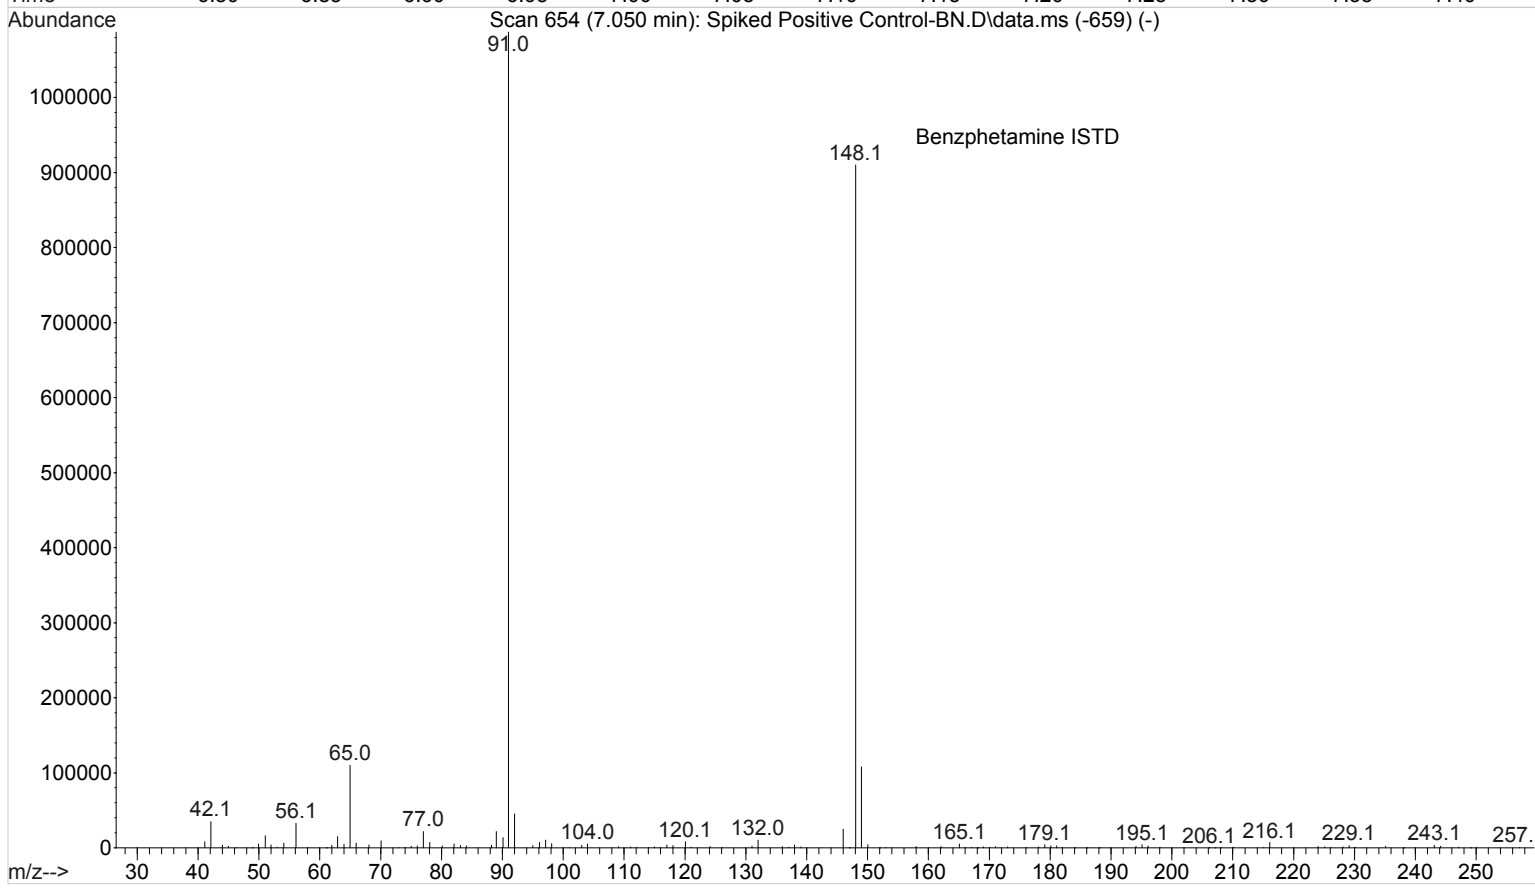
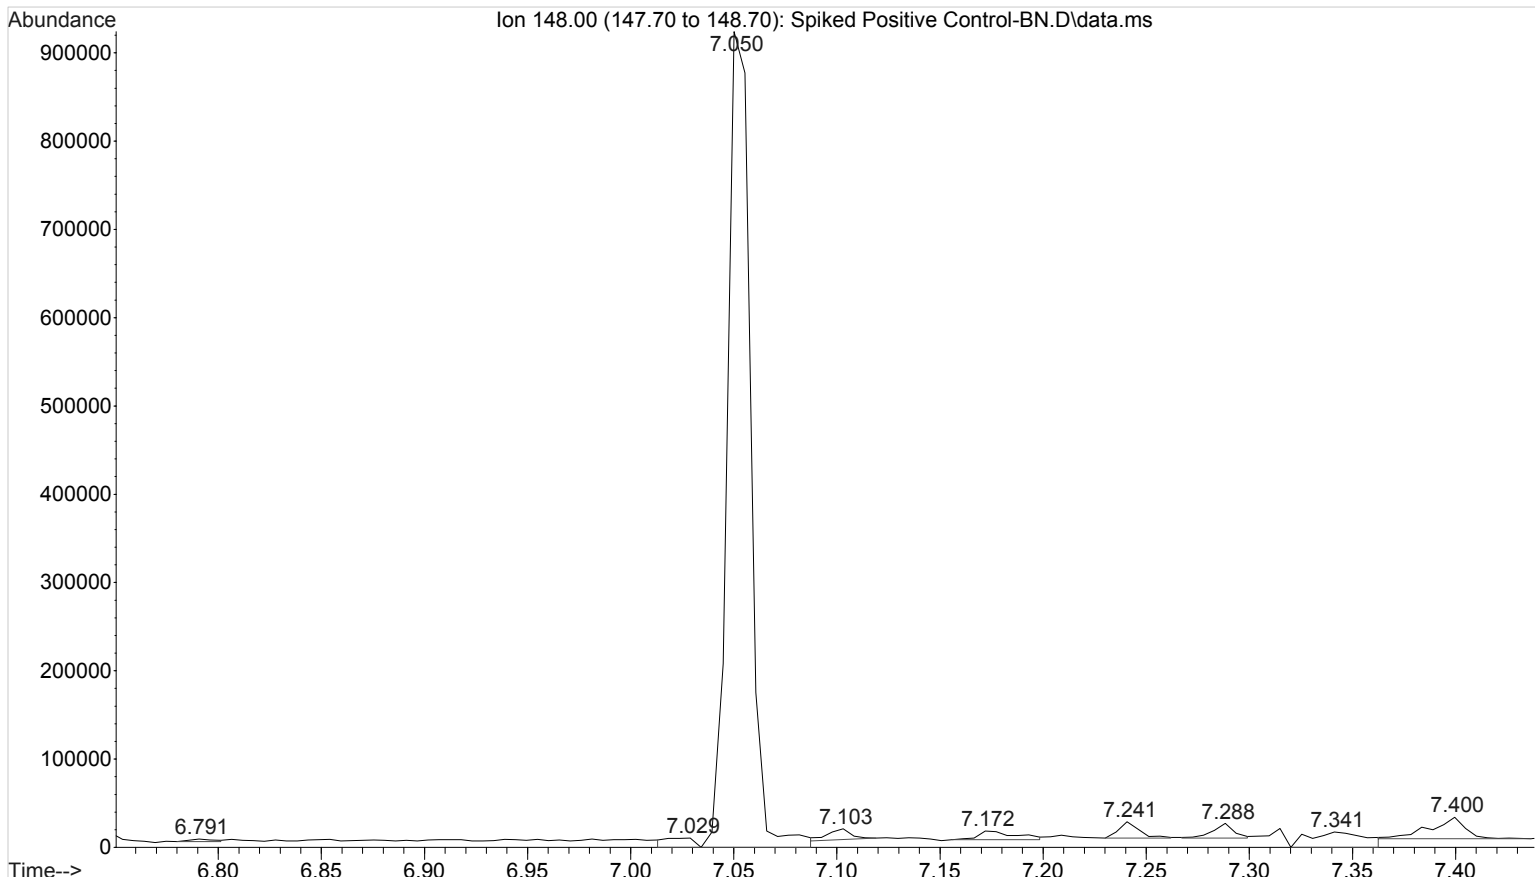


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Spiked Positive Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 16:40 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

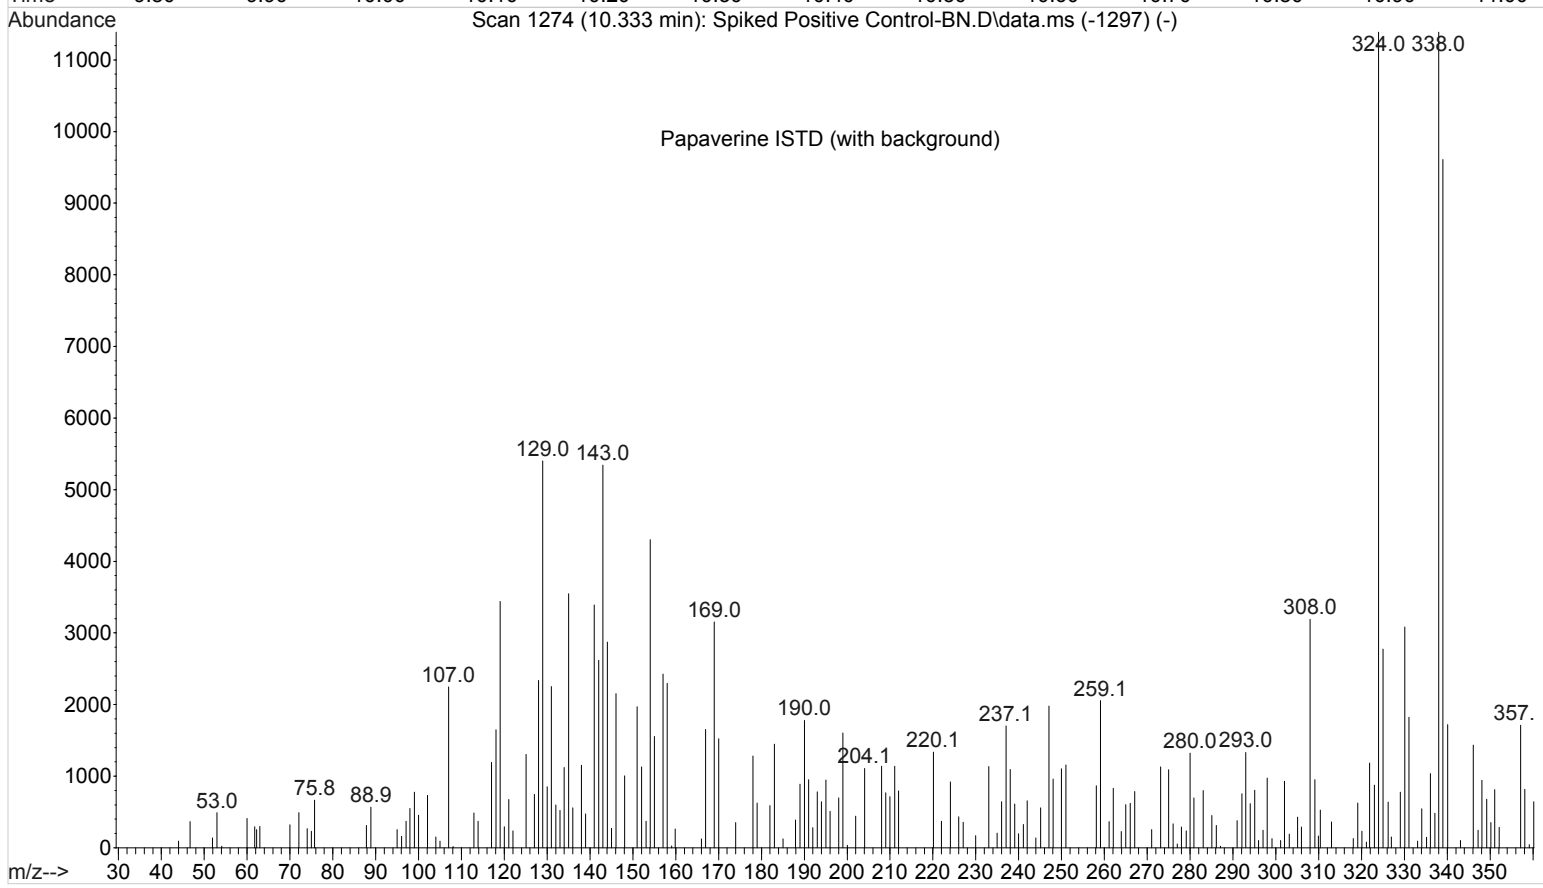
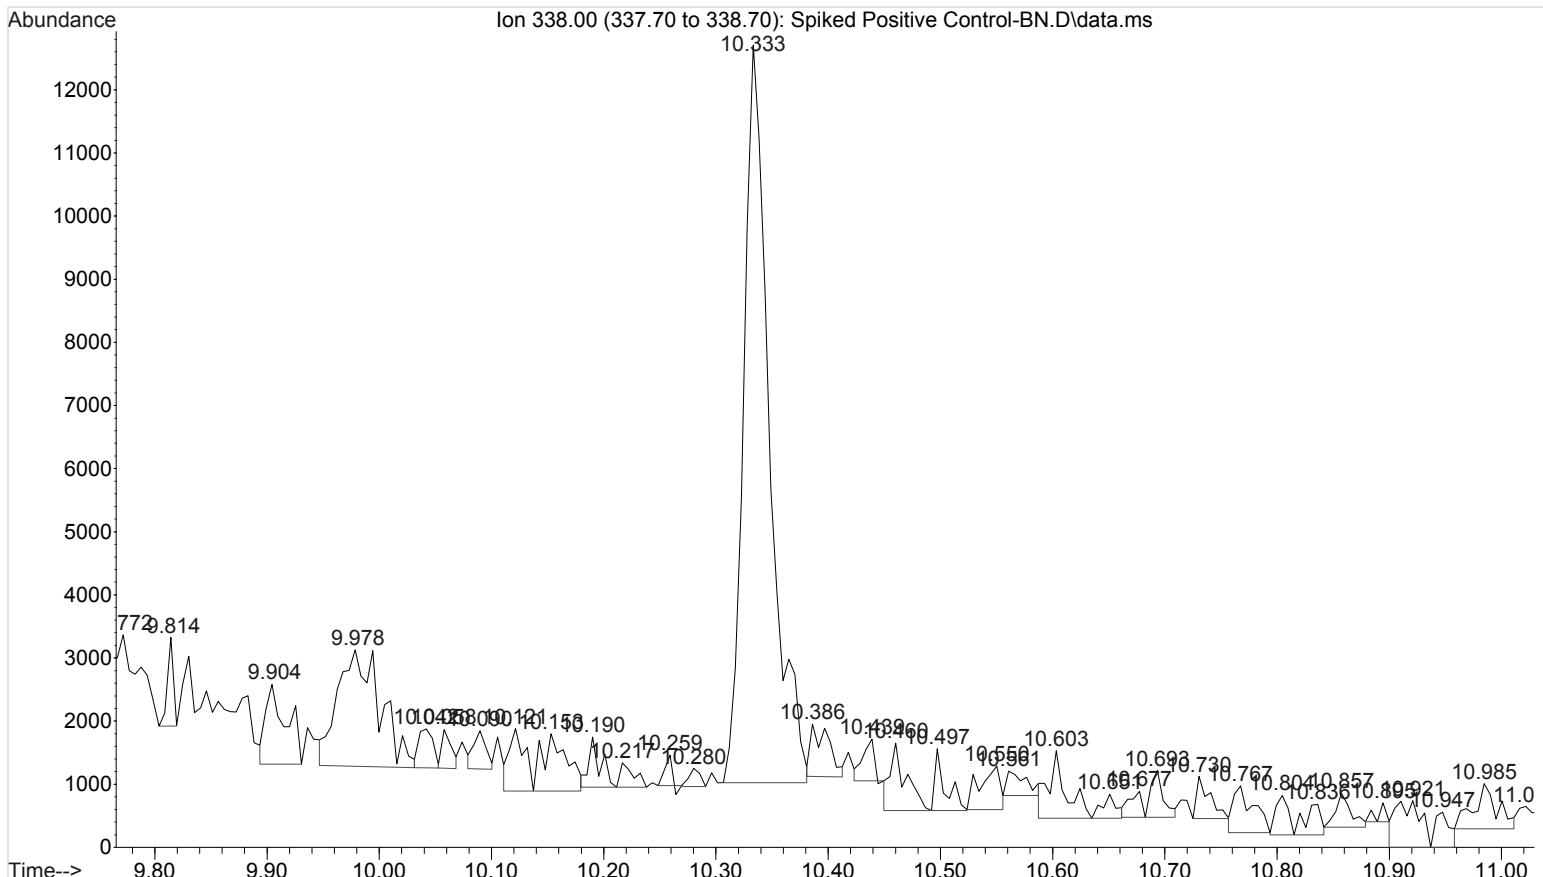


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Spiked Positive Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 16:40 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215



CS

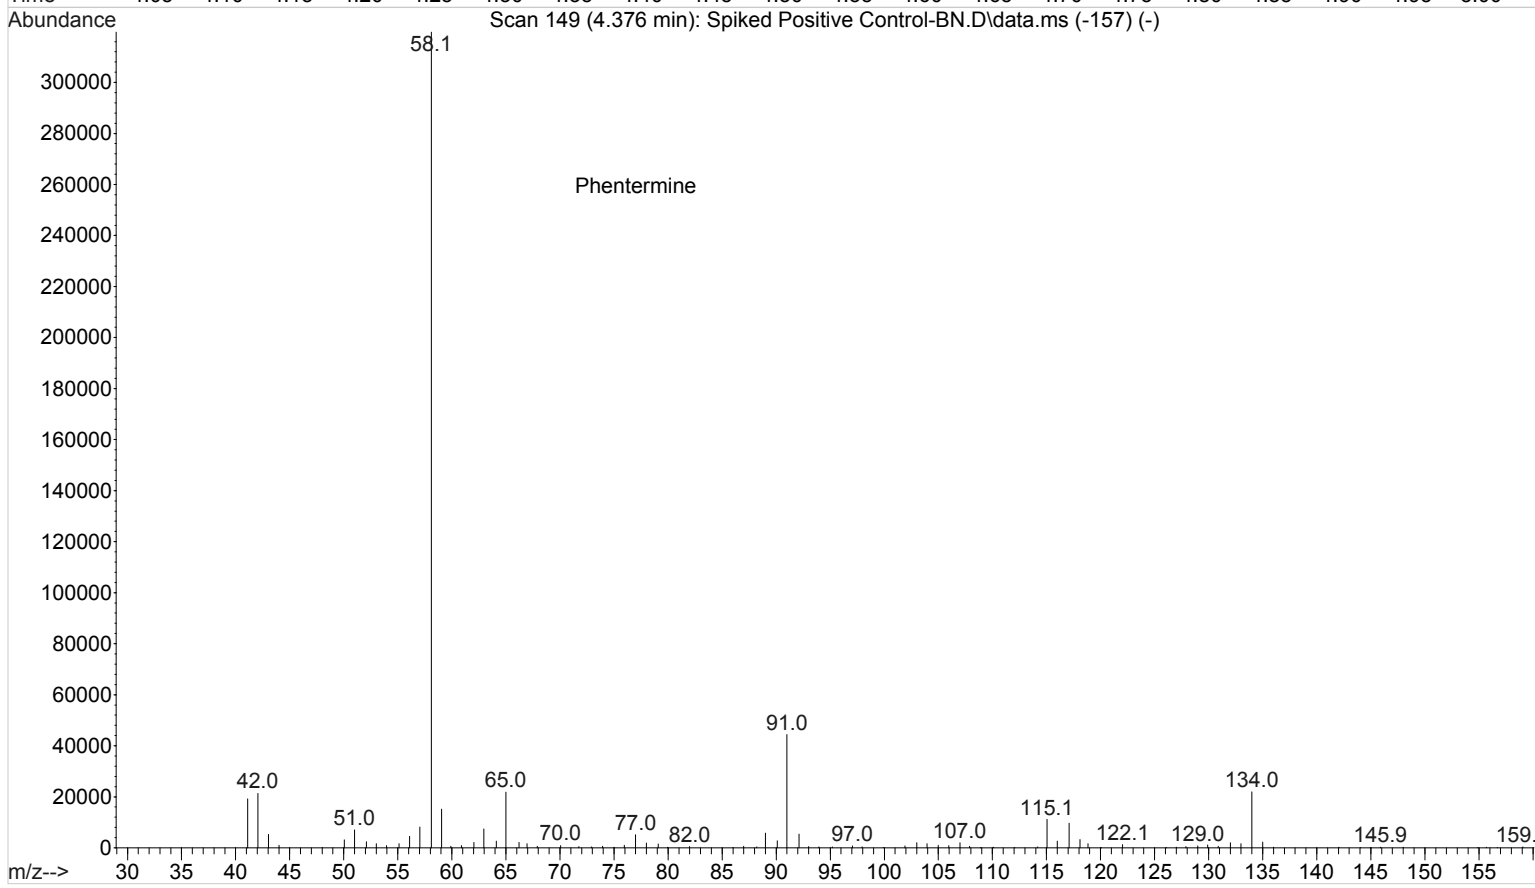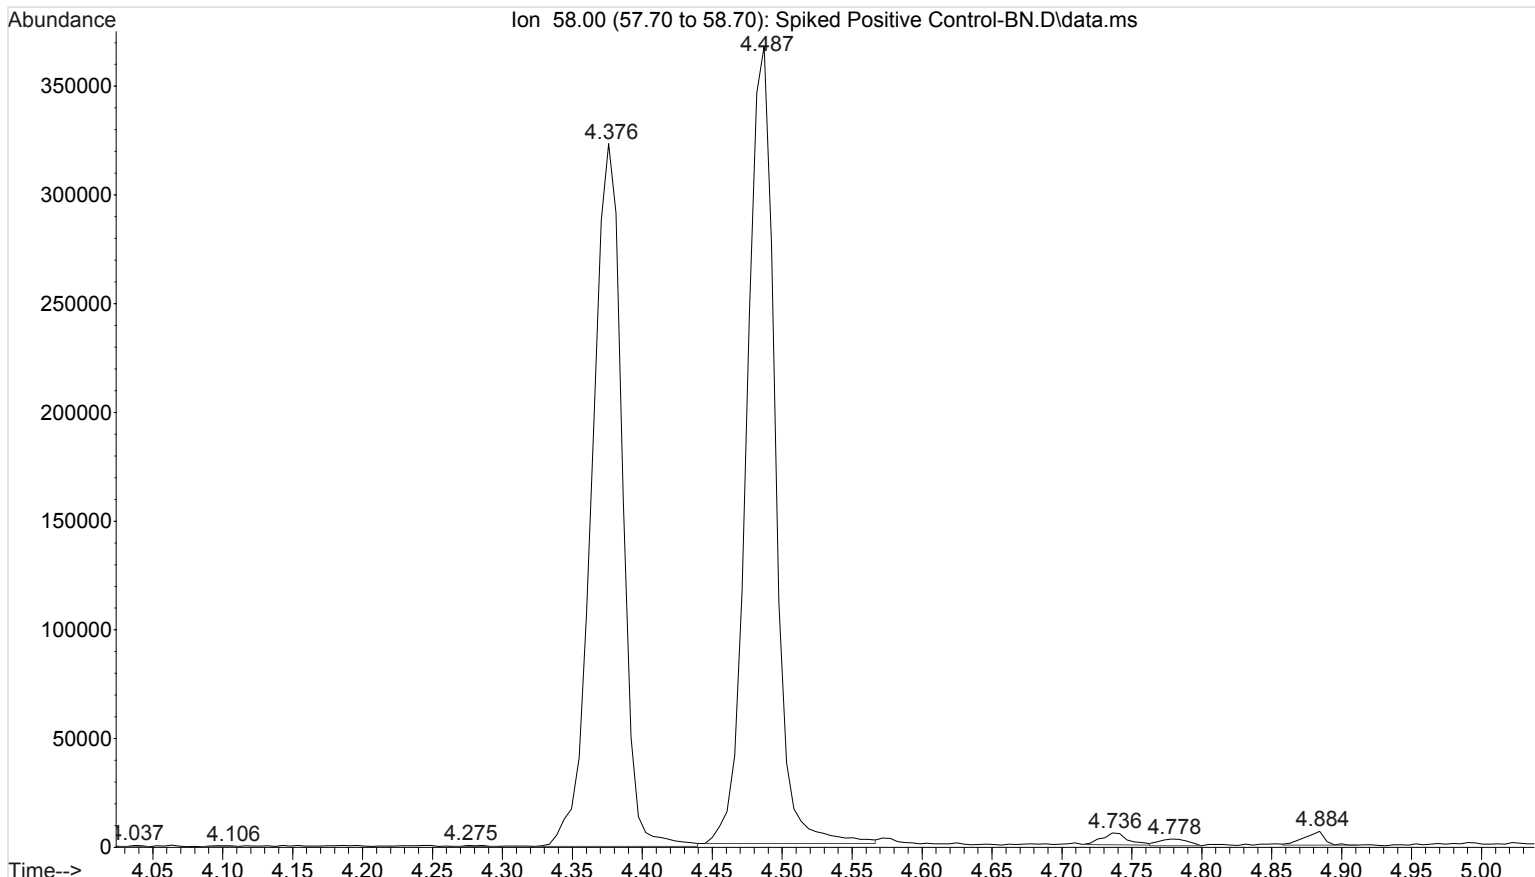

File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Spiked Positive Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 16:40 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

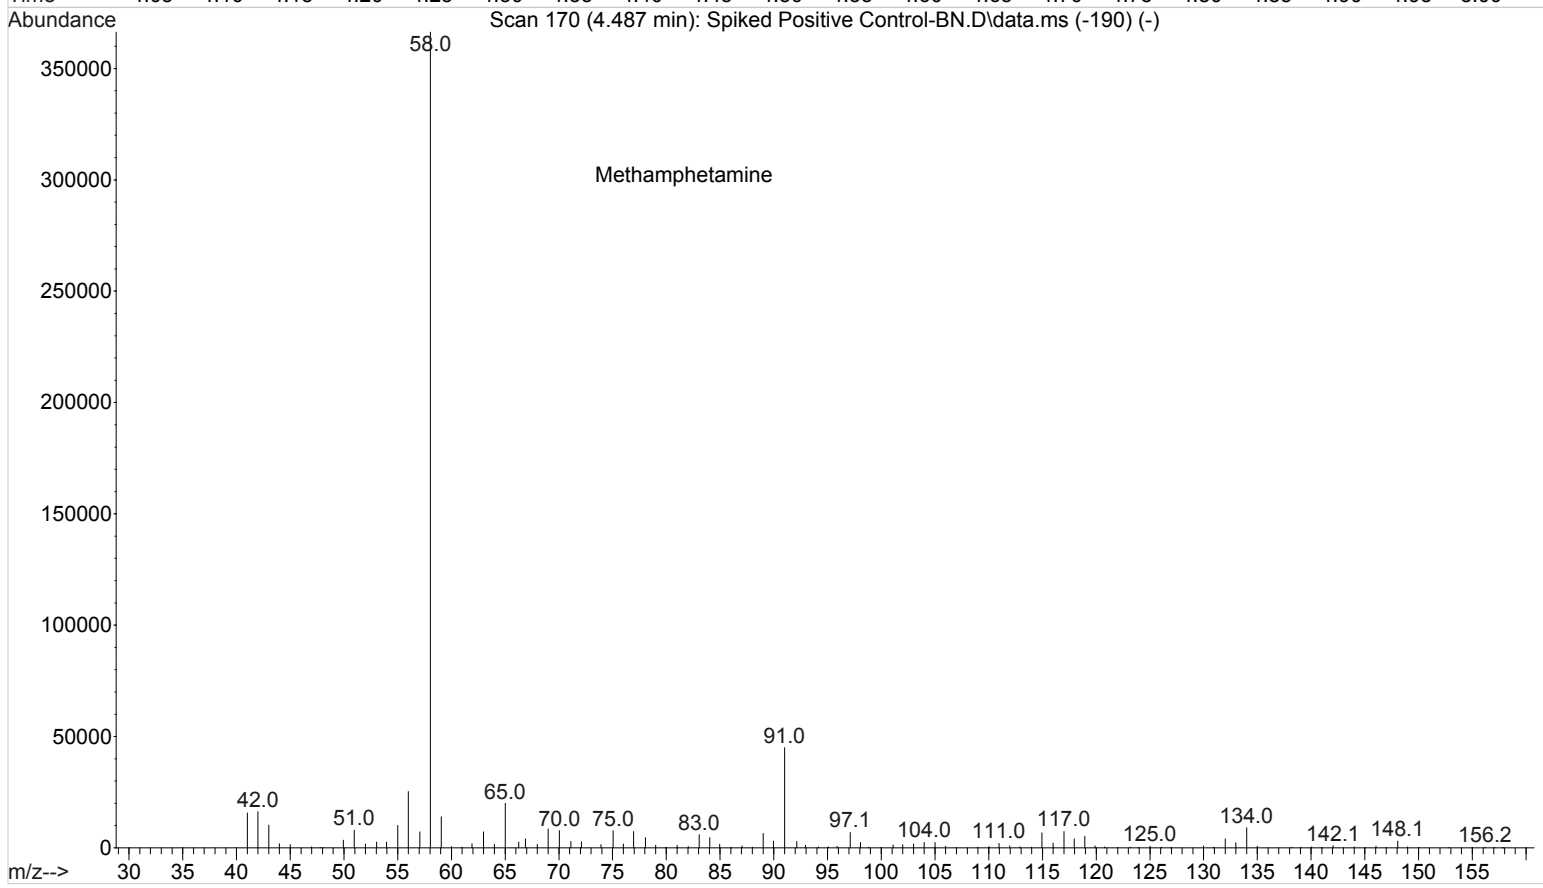
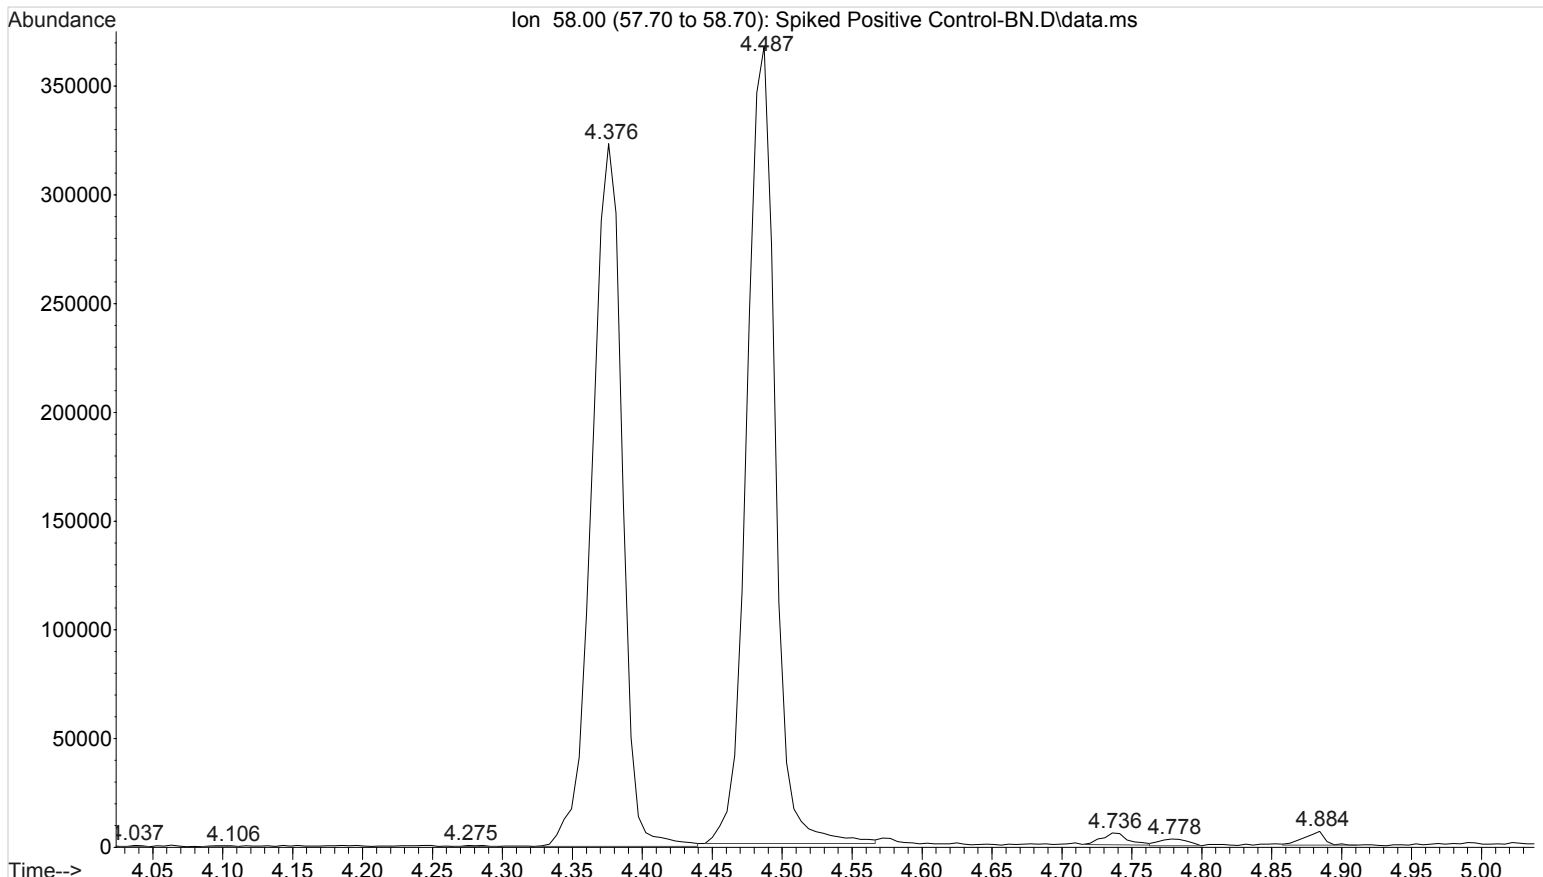


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Spiked Positive Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 16:40 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

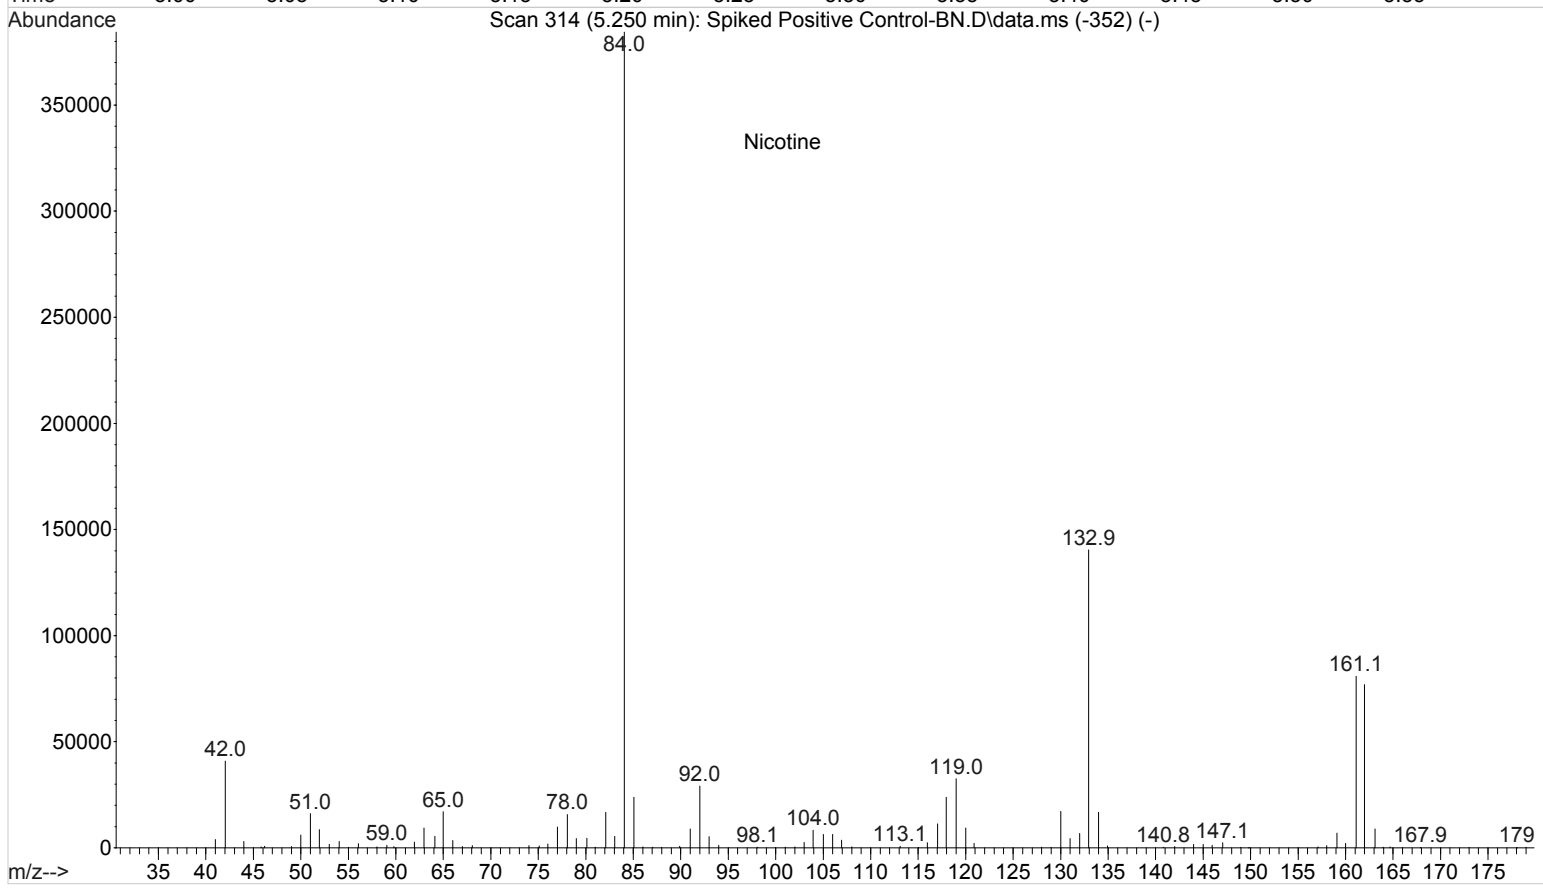
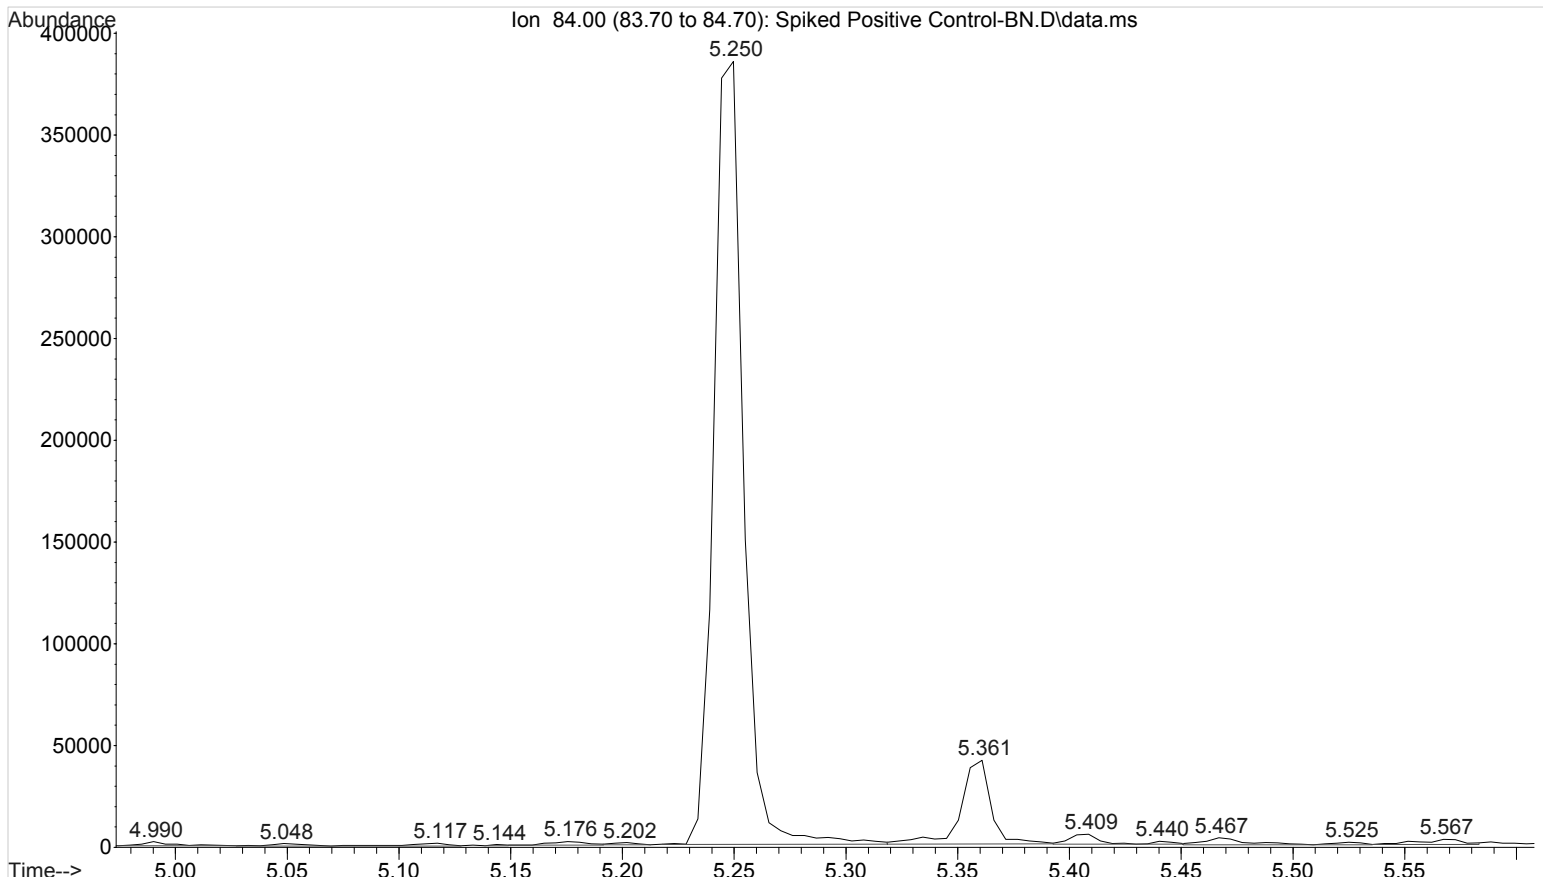


Nicotine



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Spiked Positive Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 16:40 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

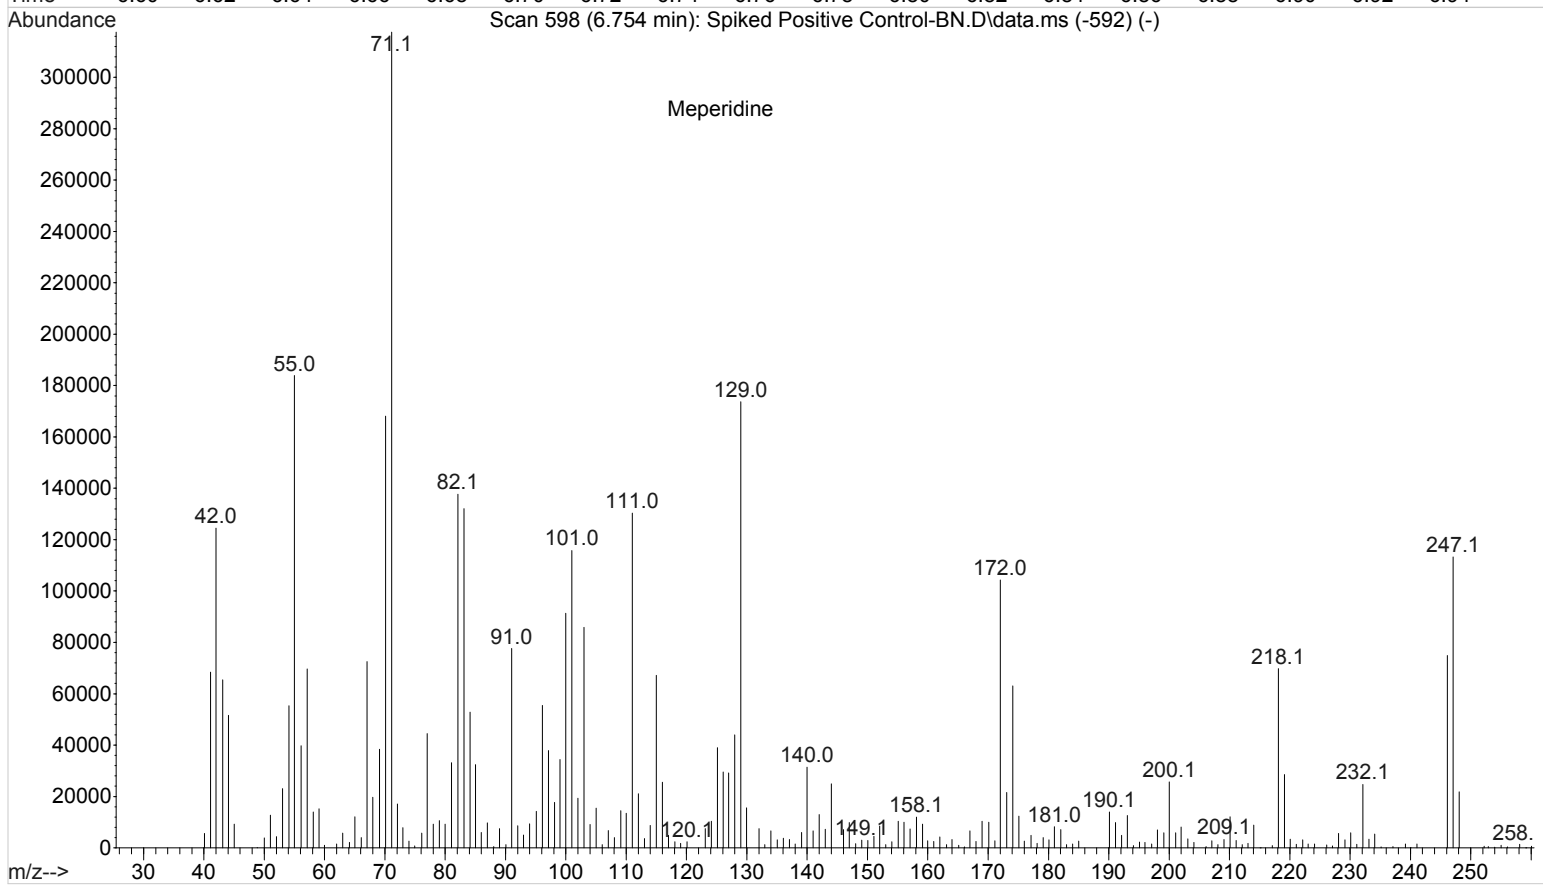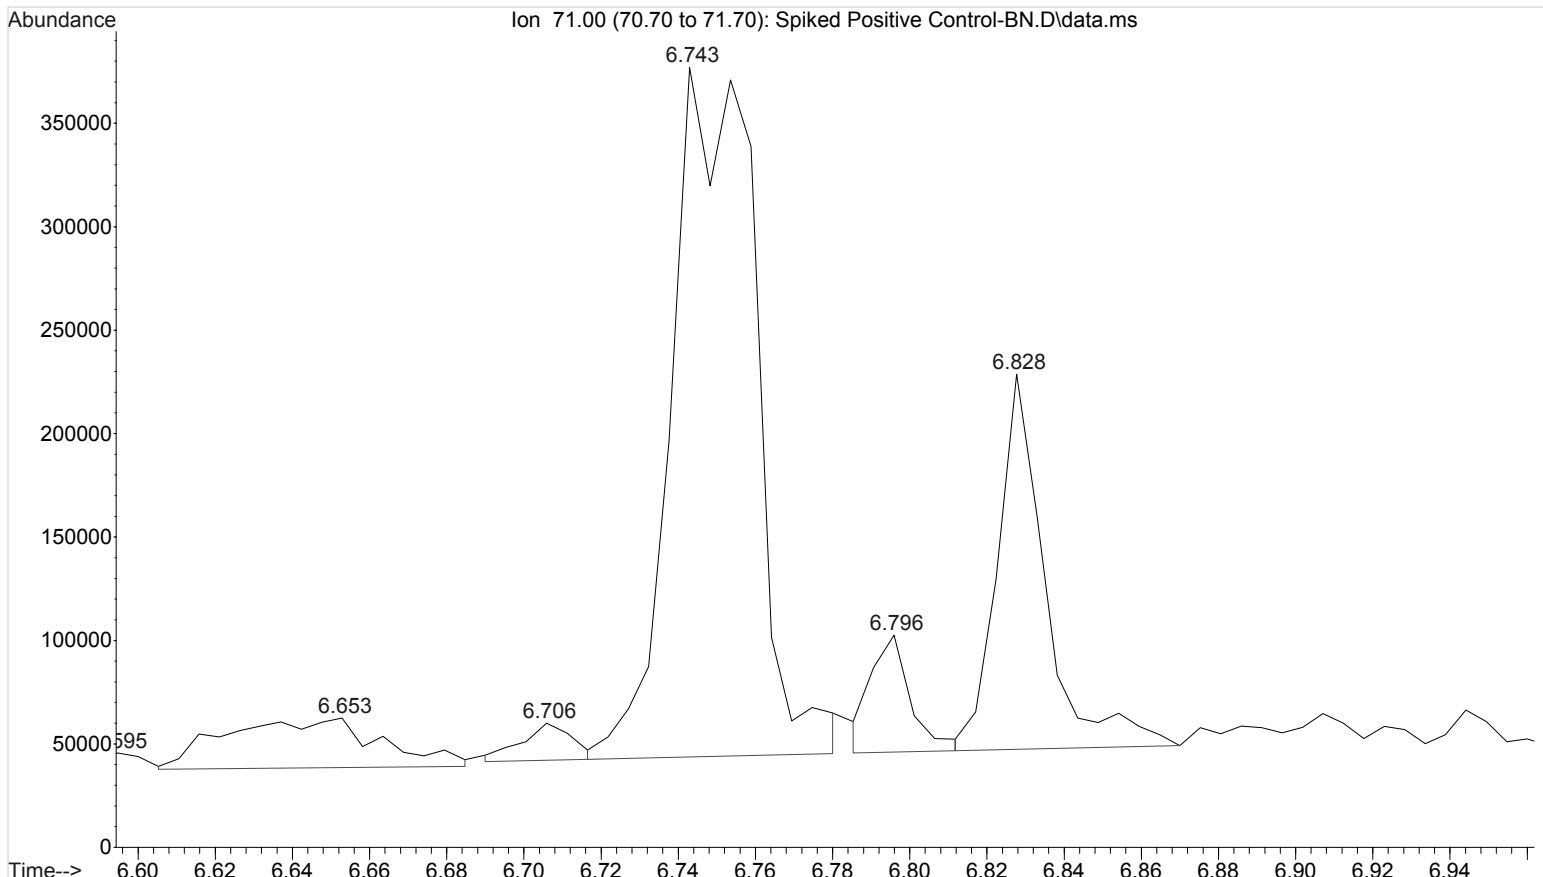



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Spiked Positive Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 16:40 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

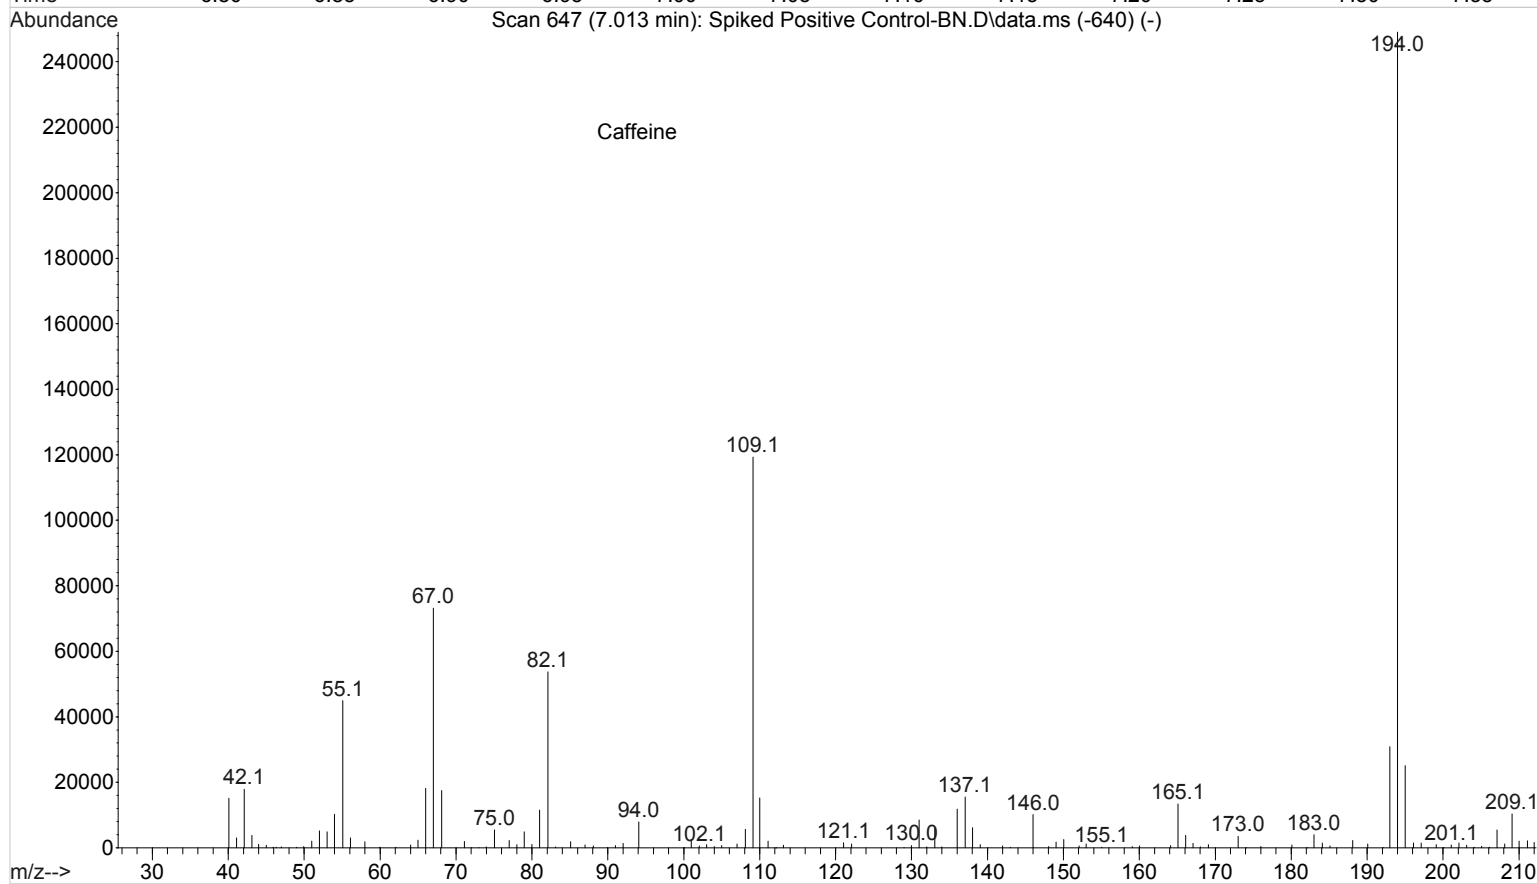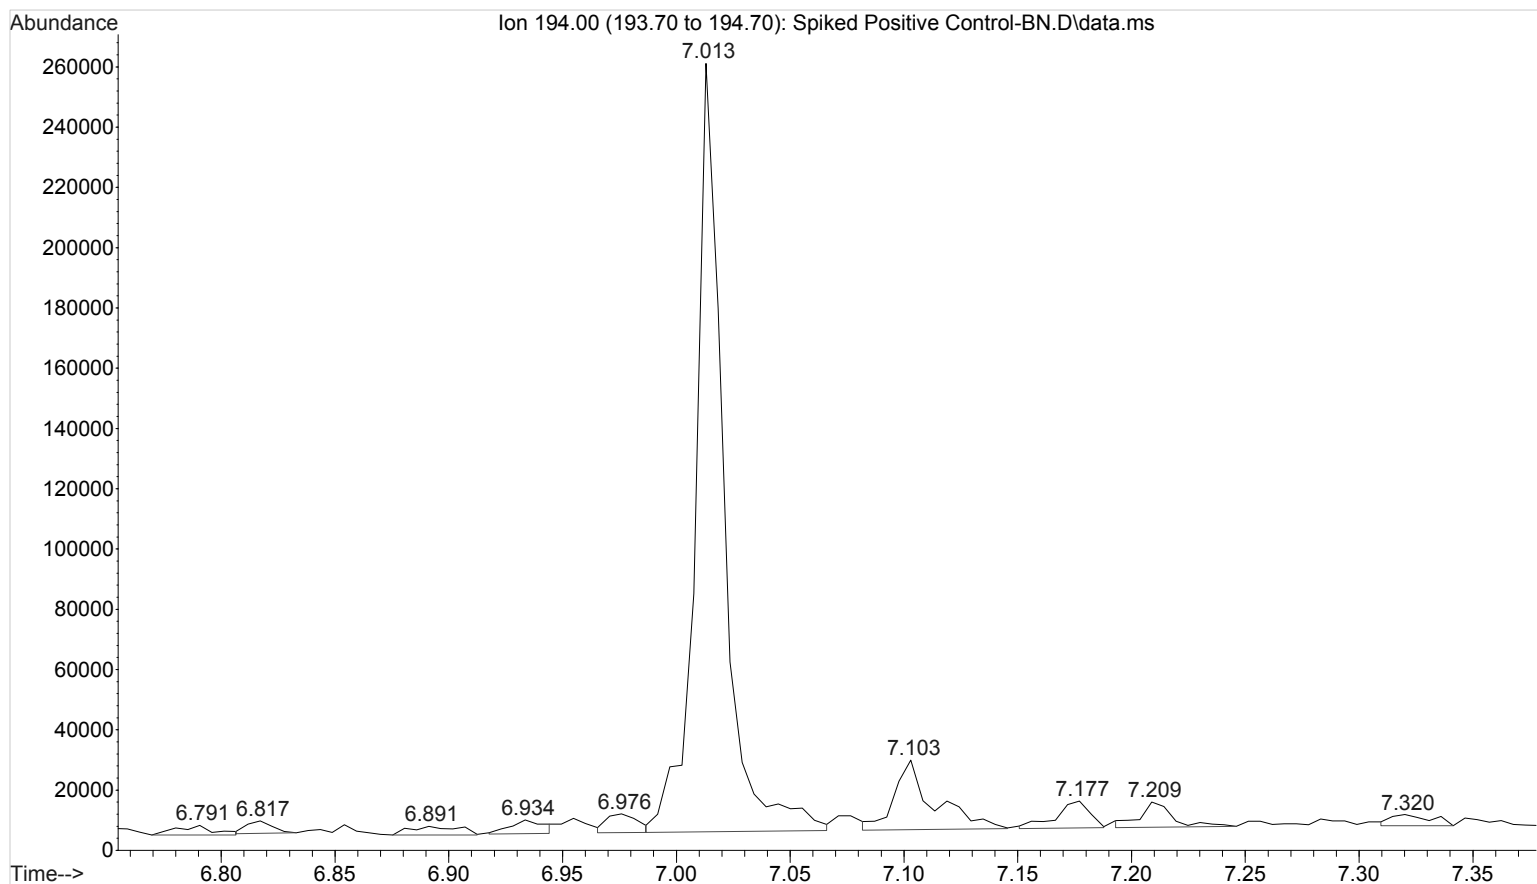



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Spiked Positive Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 16:40 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

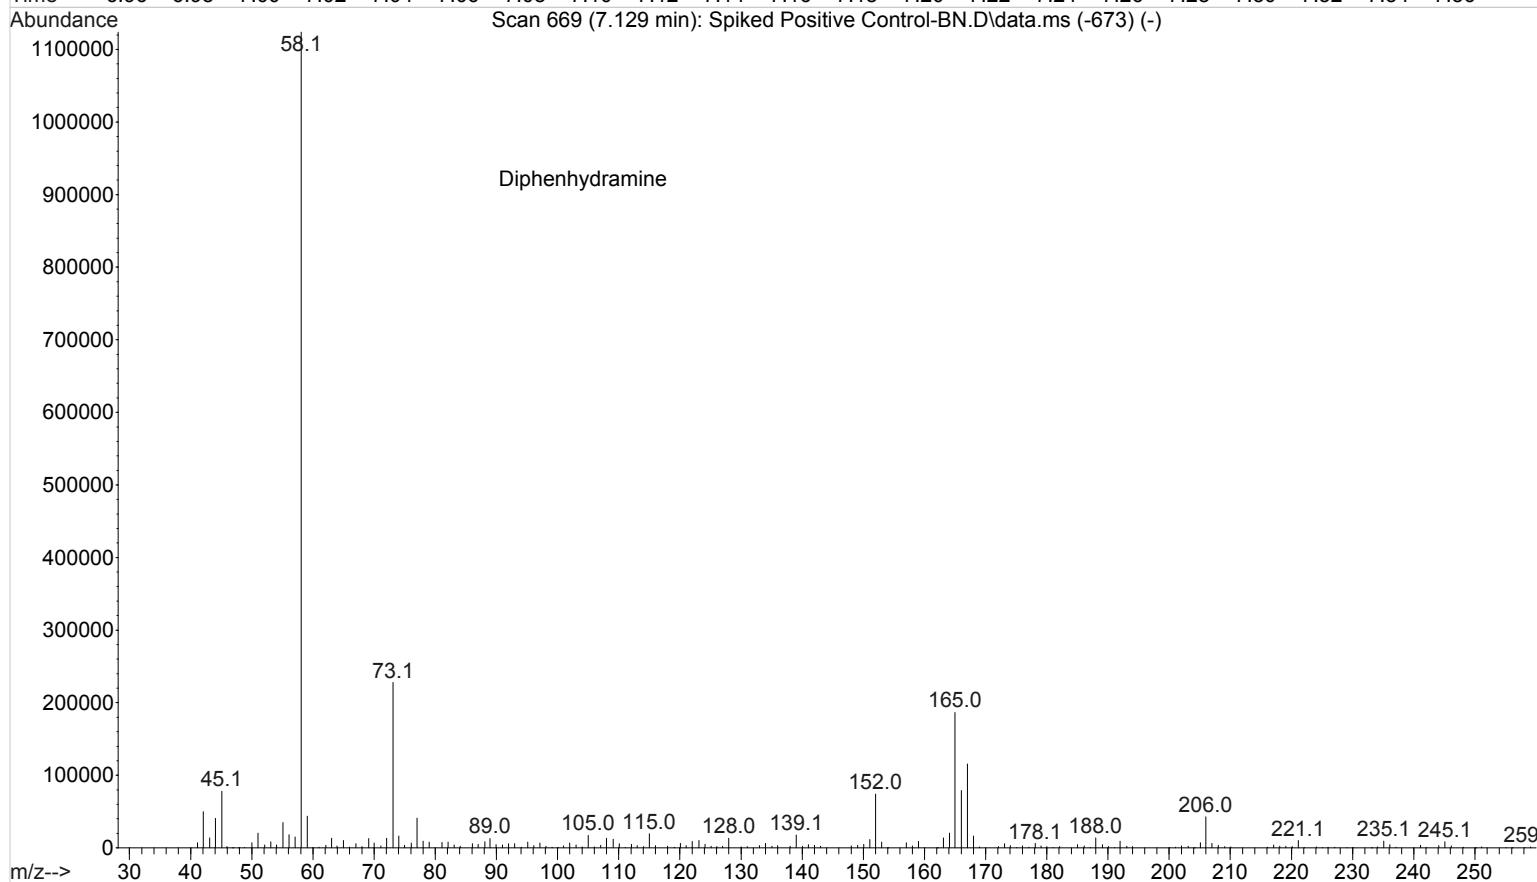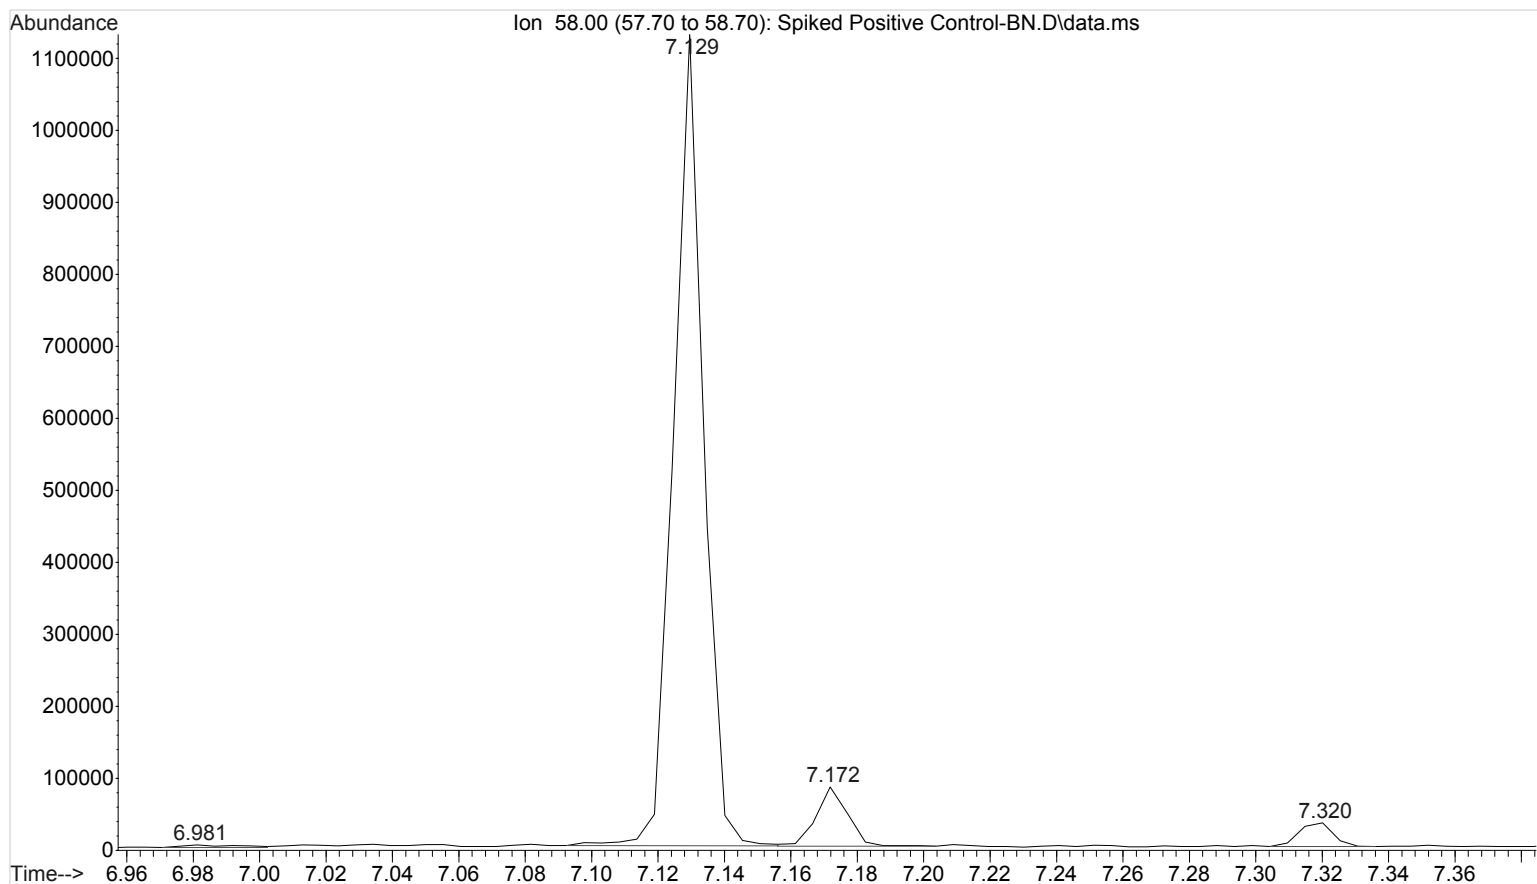



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Spiked Positive Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 16:40 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

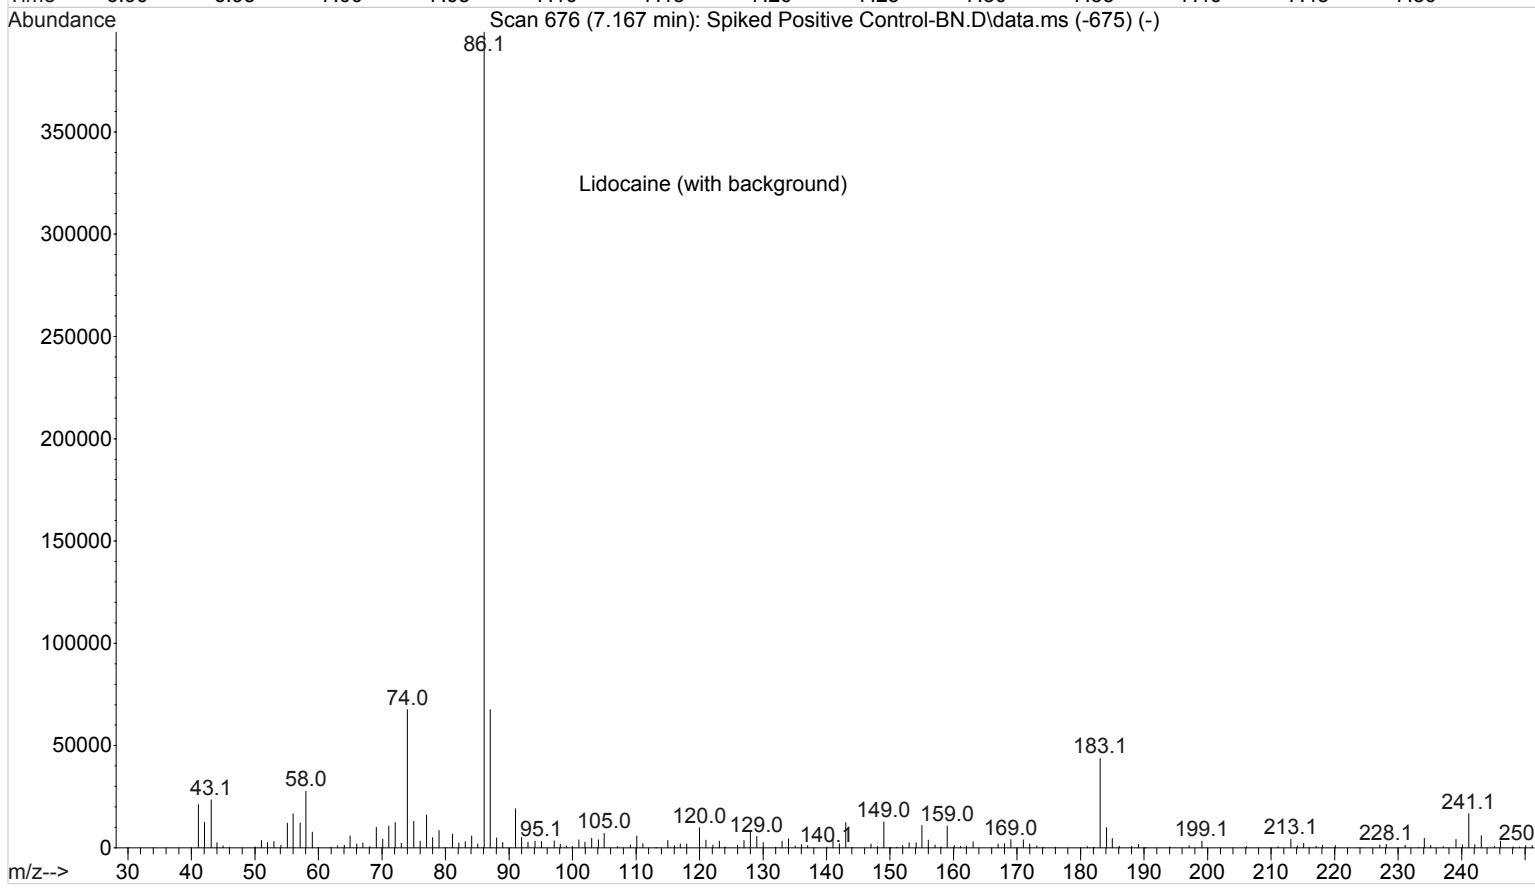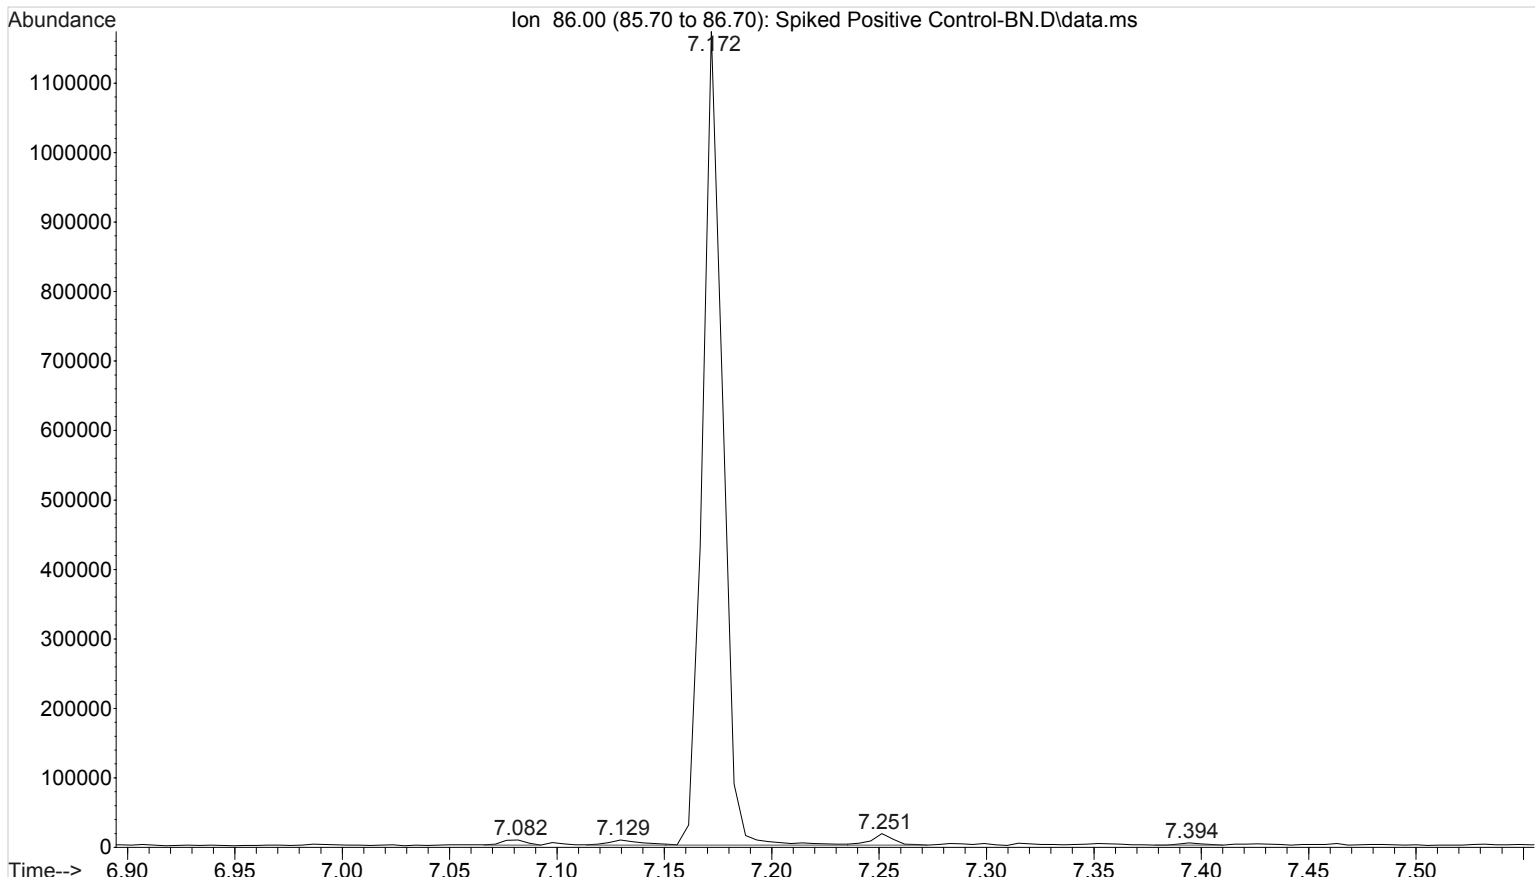



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Spiked Positive Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 16:40 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

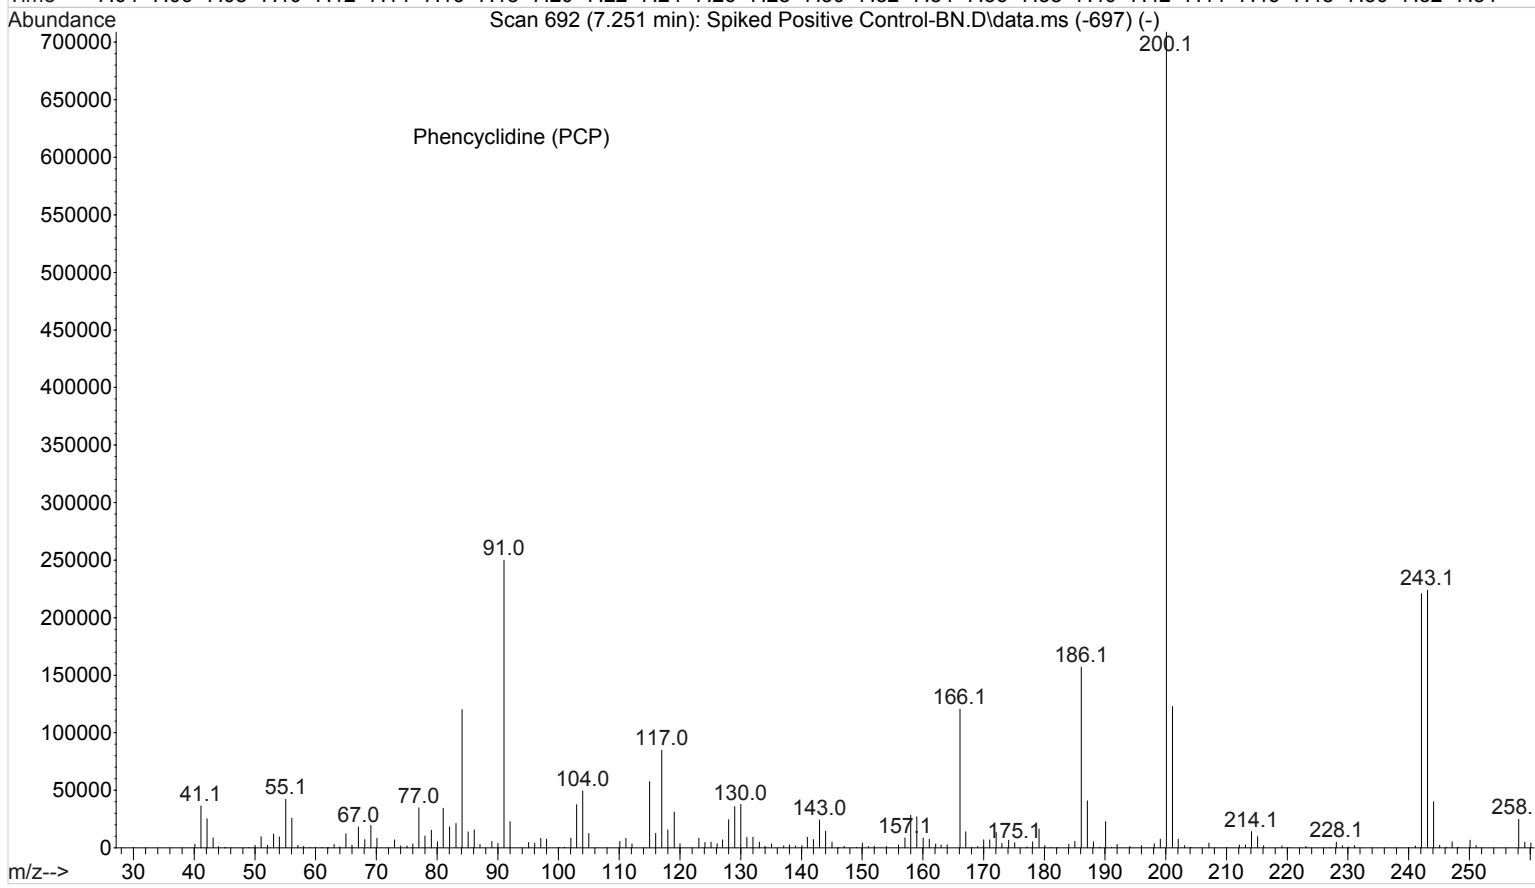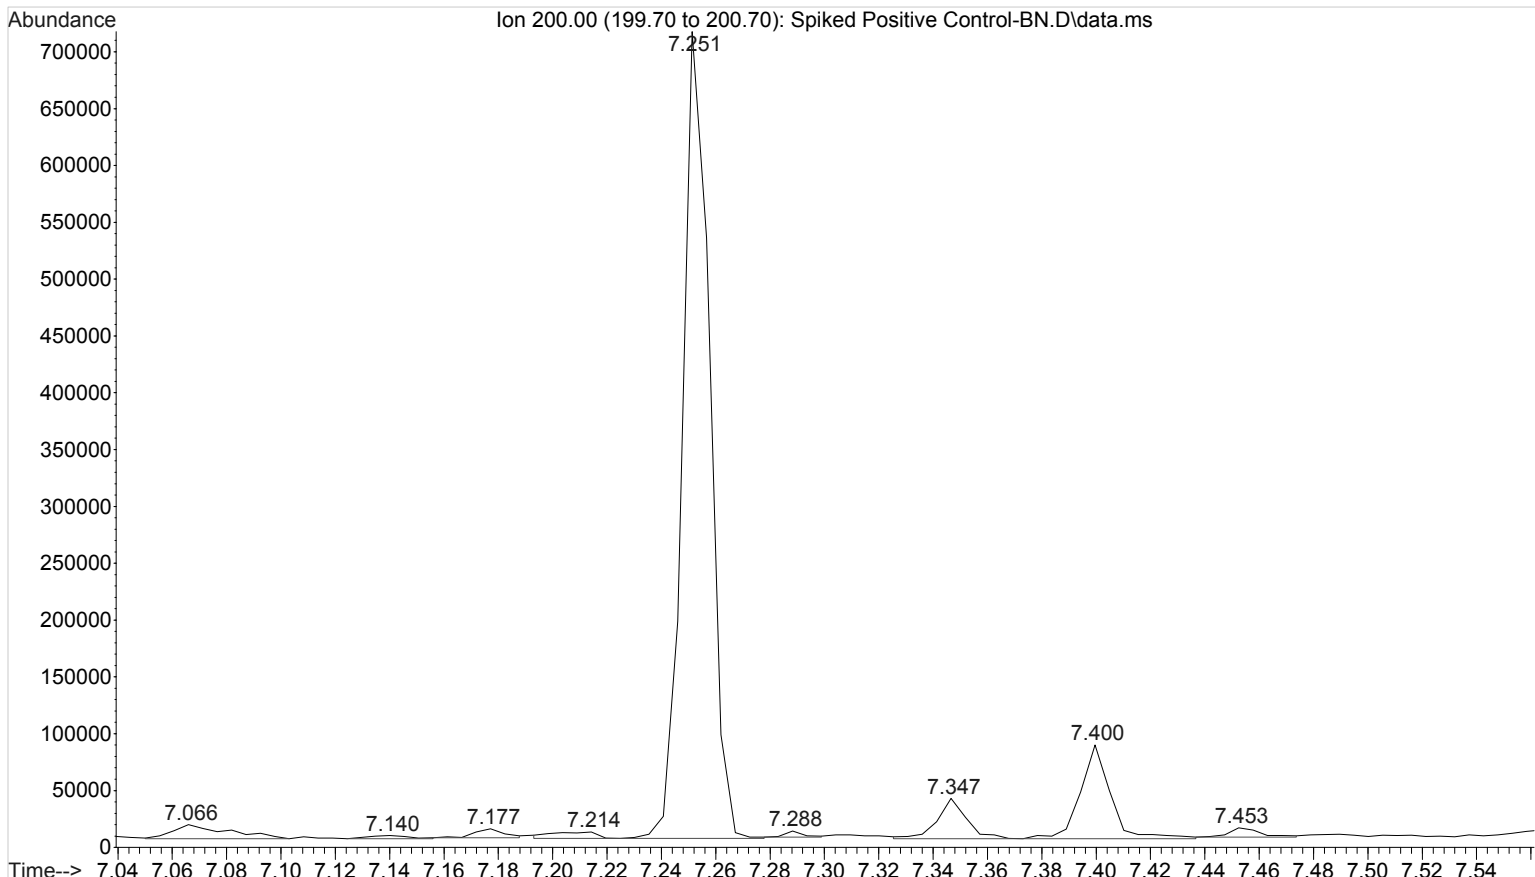

File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Spiked Positive Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 16:40 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

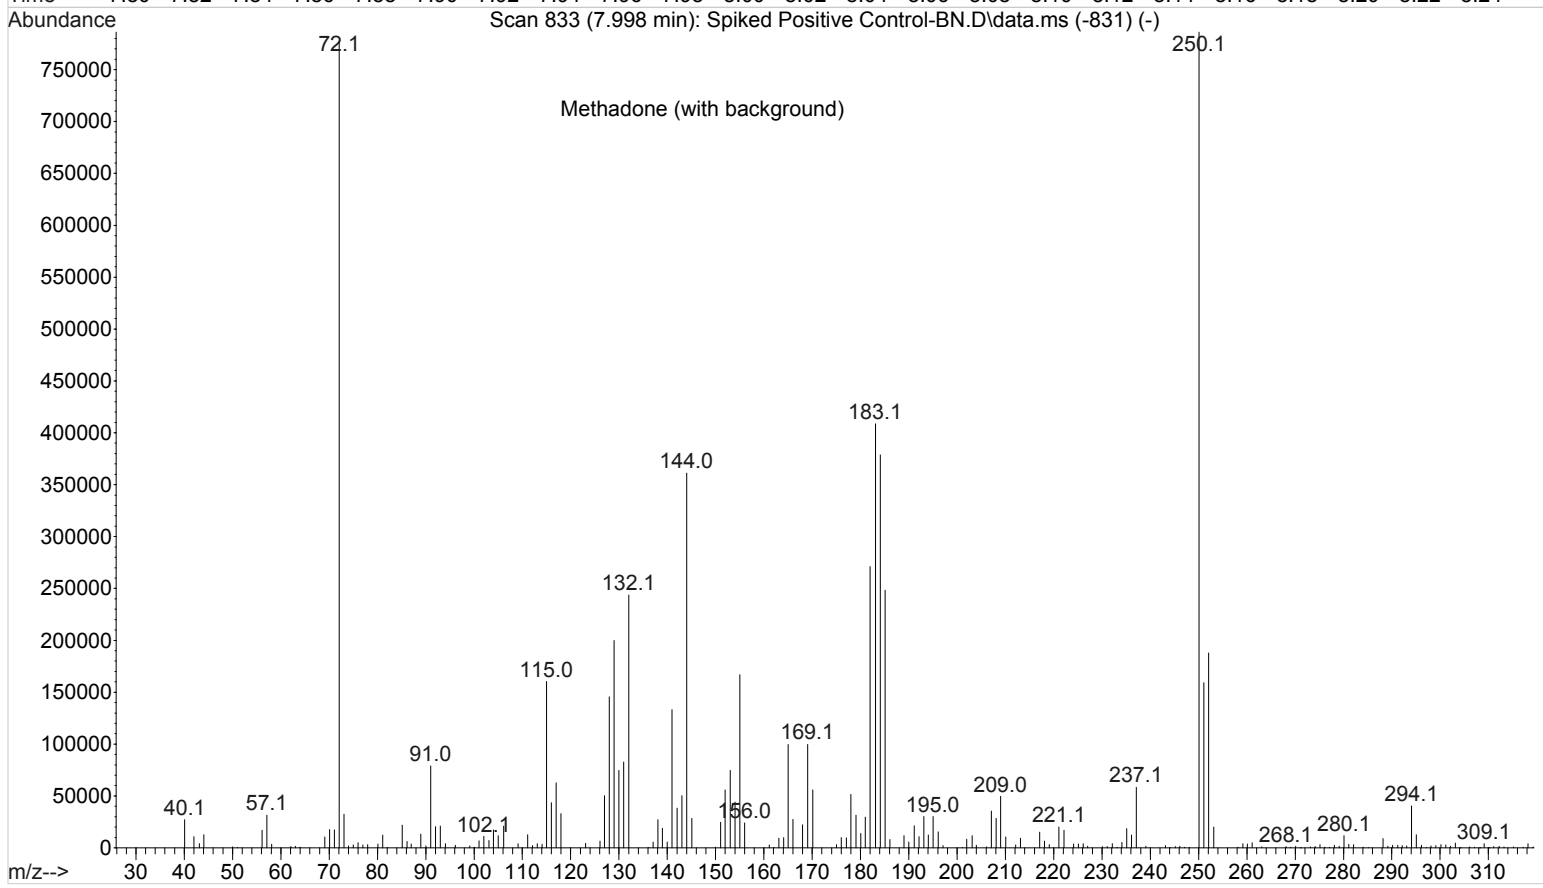
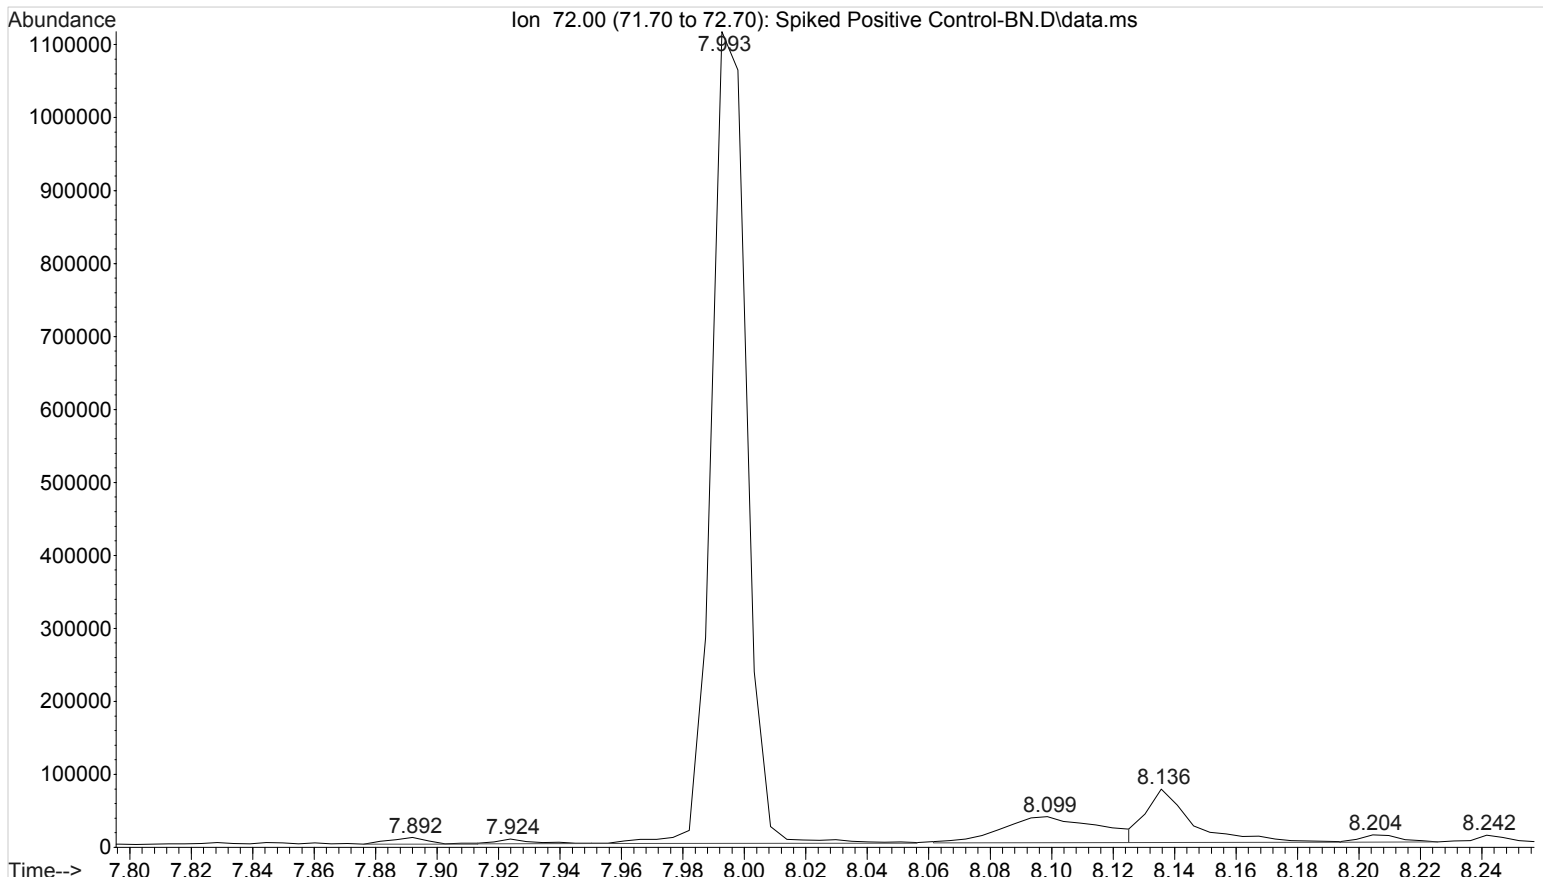


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Spiked Positive Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 16:40 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

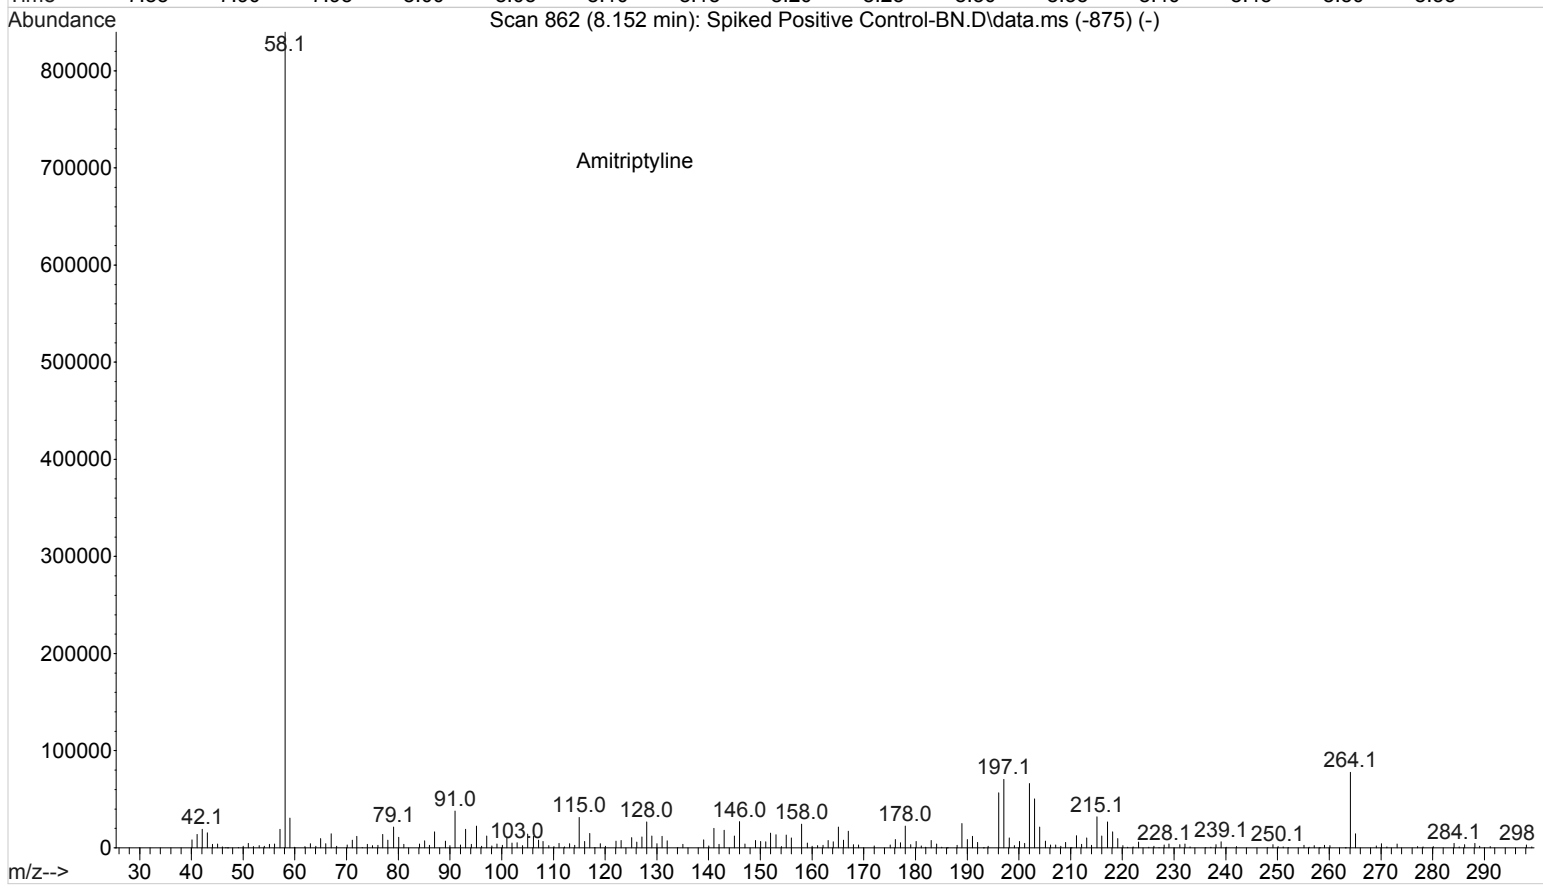
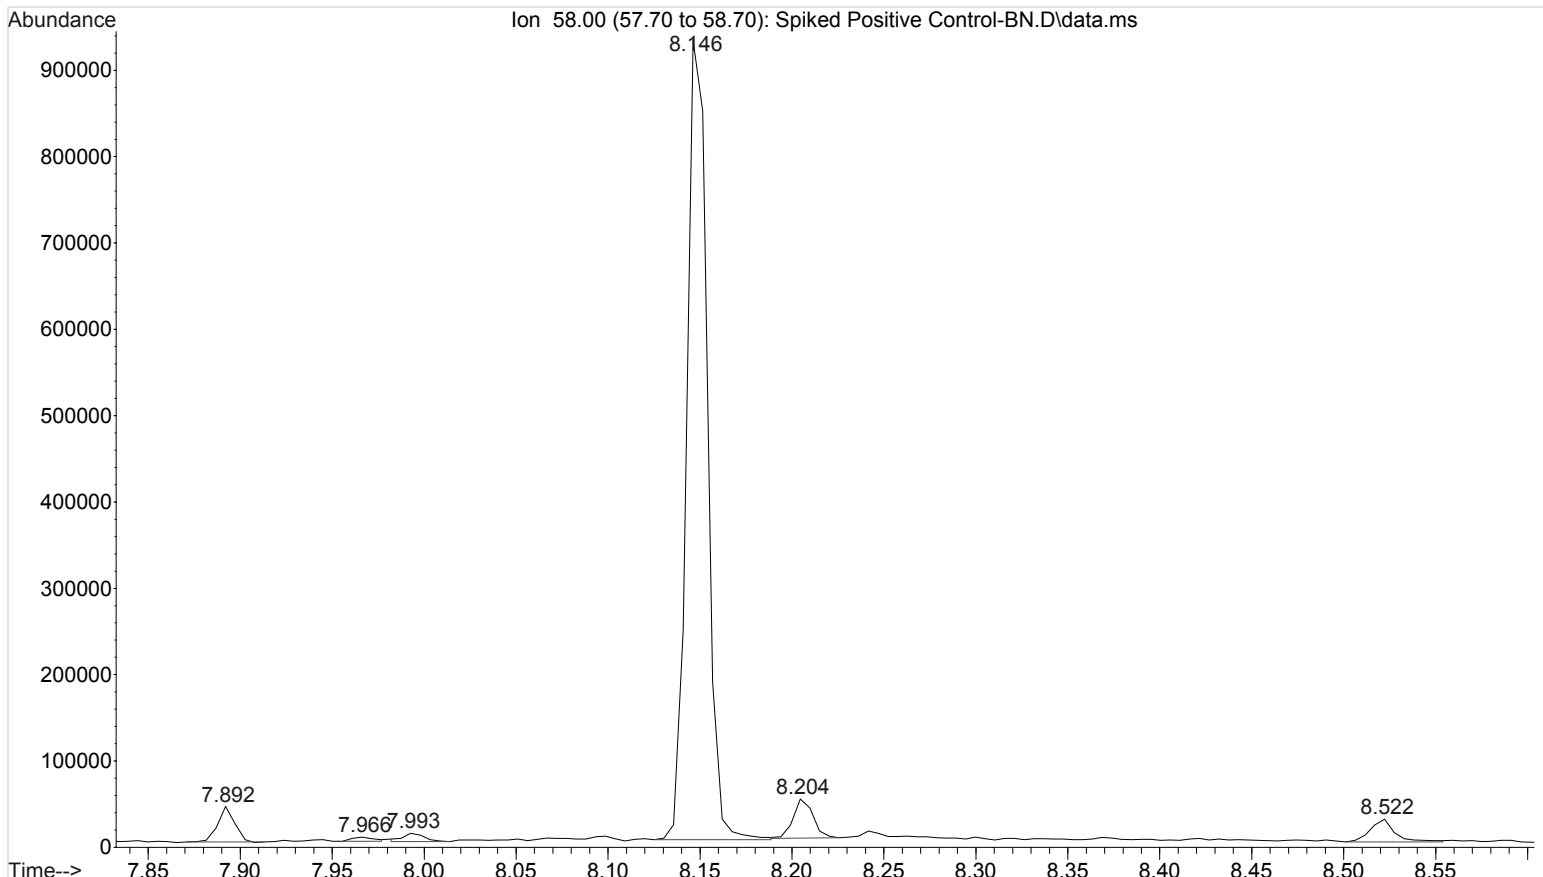


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Spiked Positive Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 16:40 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

9

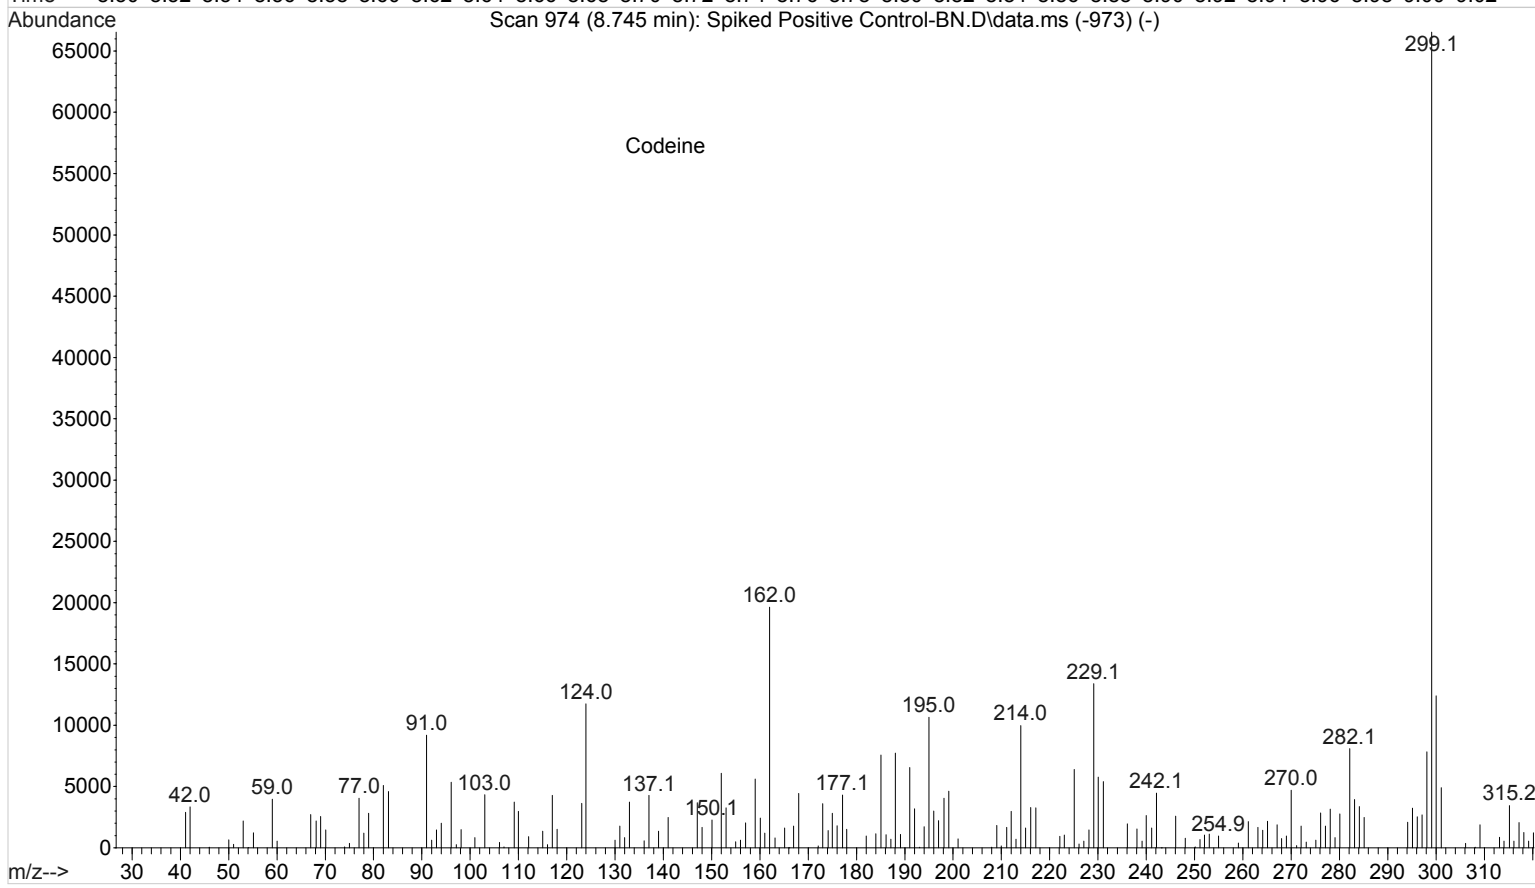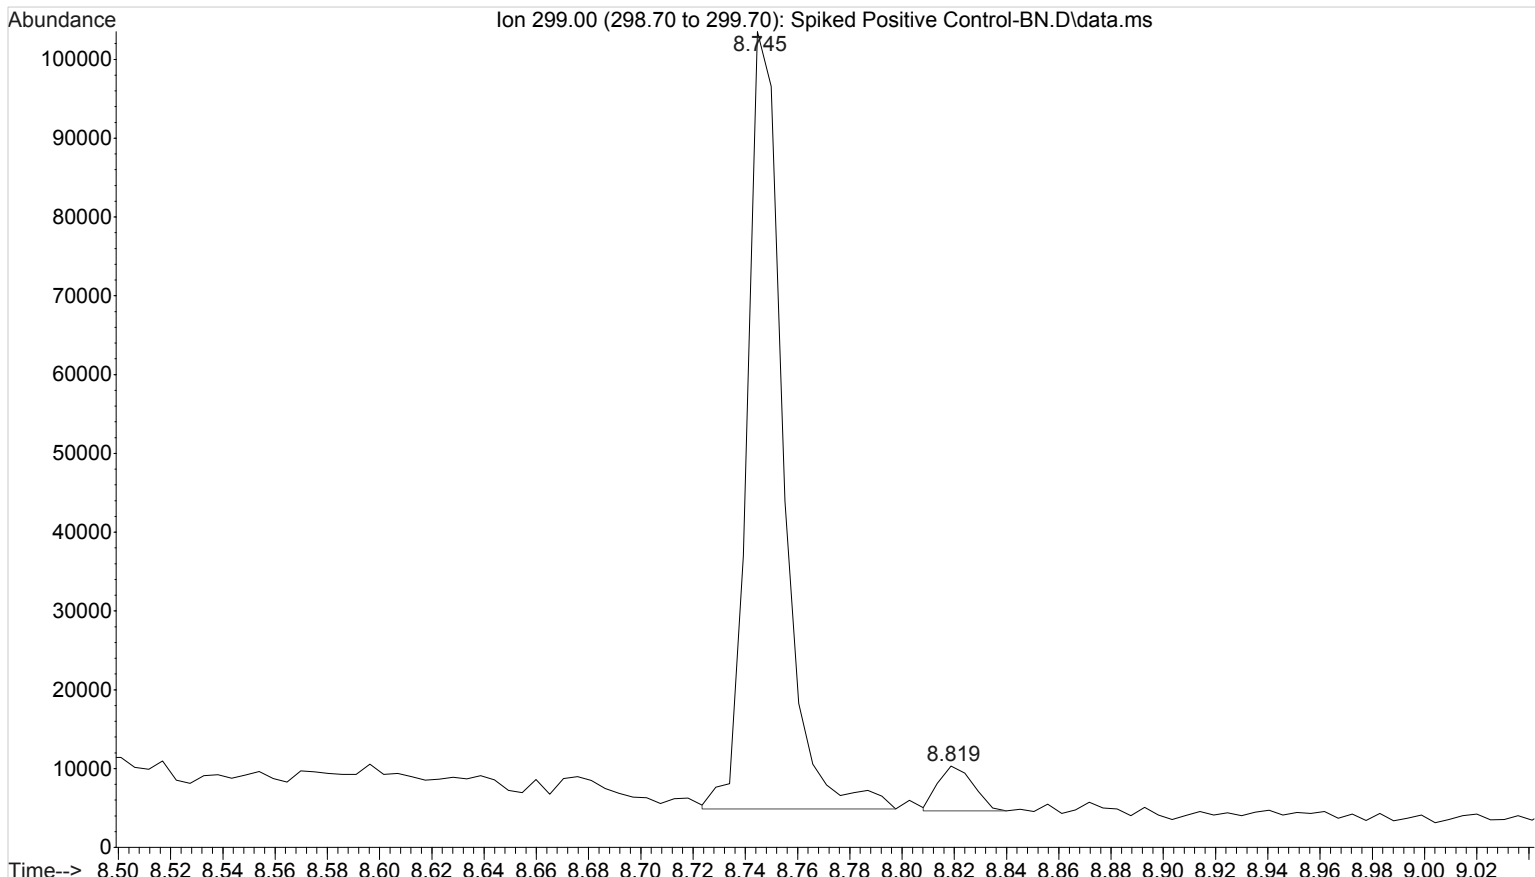

File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Spiked Positive Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 16:40 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

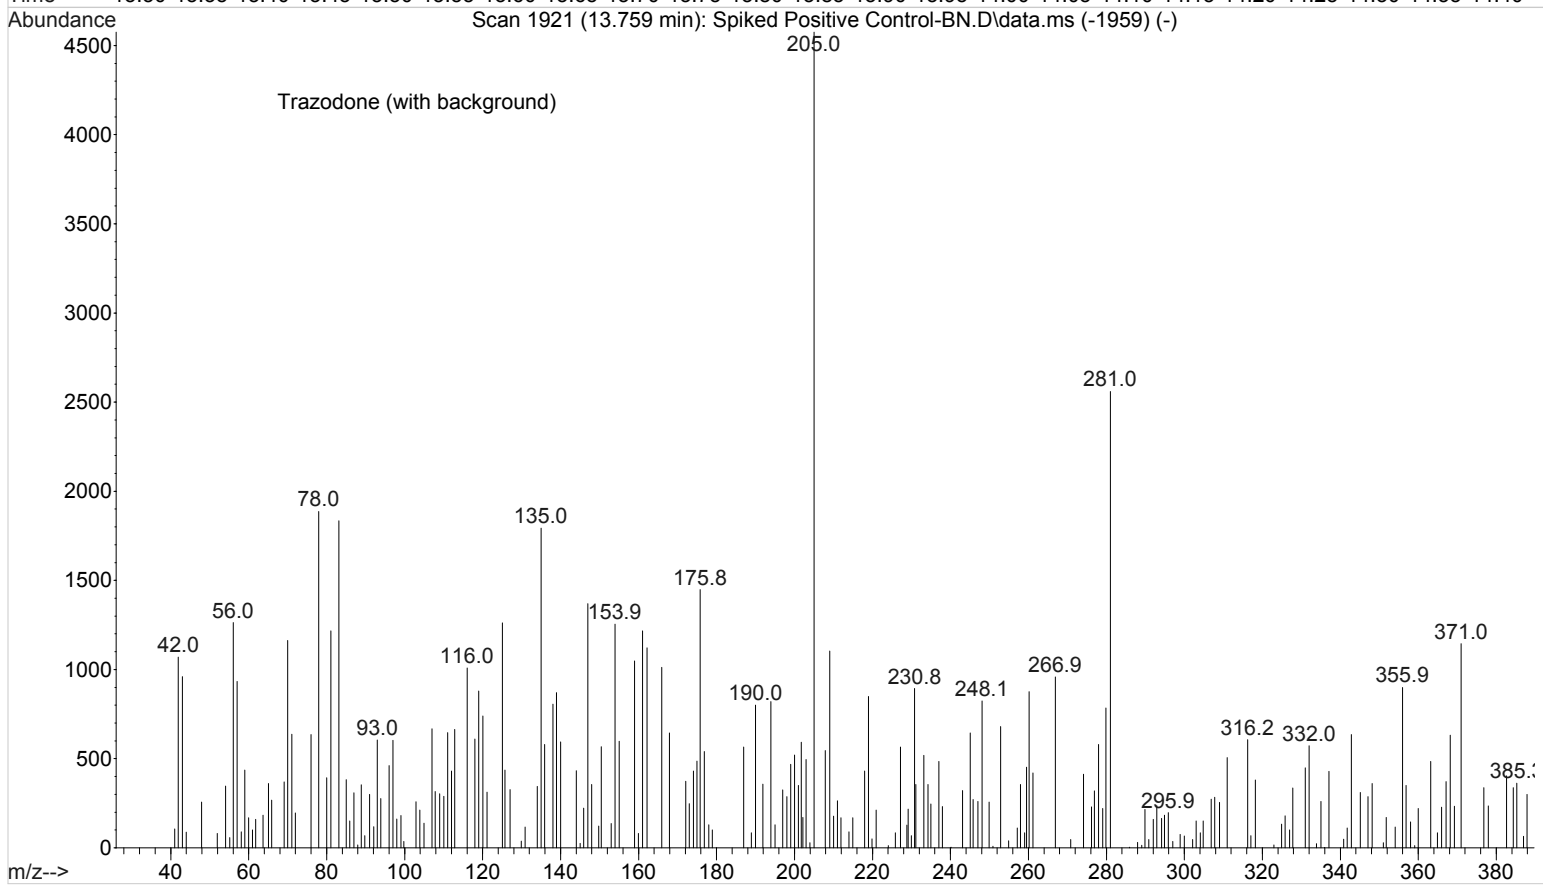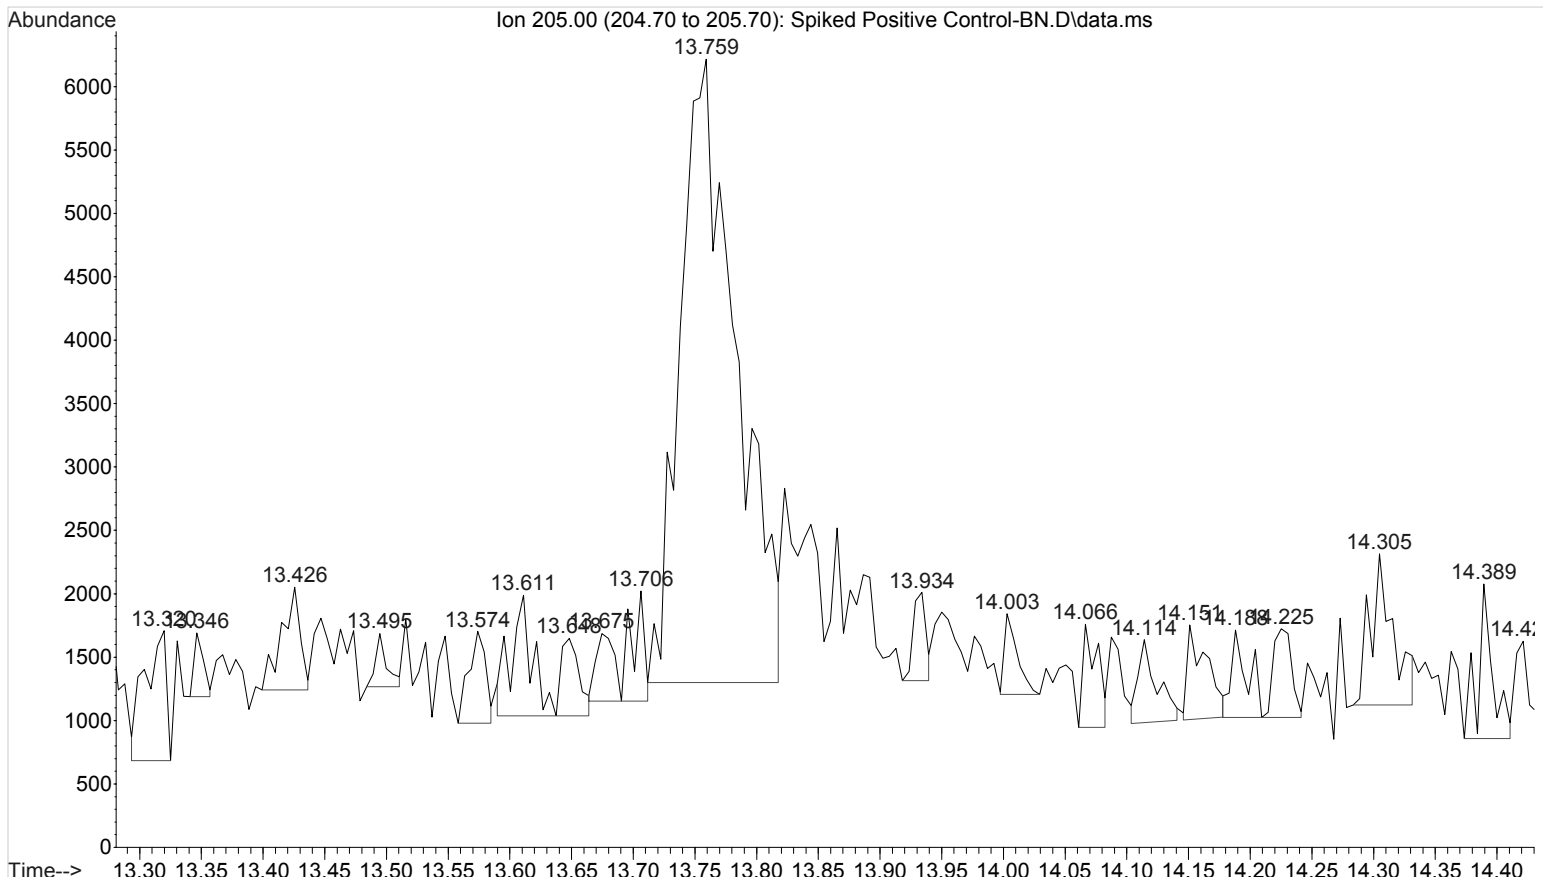

Analytical Method 3.6.1 & 3.6.7 QA Check List

Run Start Date: 07/14/2016

Analyst: CS

(Long GC/MS temperature program)

Positive Control Compound List


- Phentermine
- Methamphetamine
- Nicotine
- Meperidine
- Caffeine
- Diphenhydramine
- Lidocaine
- PCP
- Methadone
- Amitriptyline
- Codeine
- Trazodone

Internal Standards


- Benzphetamine
- Papaverine

Optional back extraction **not** performed.
Reconstituted in MeOH.


File :I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Prerun Solvent Blankr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 17:26 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Pre-run Solvent Blank
Misc Info : Chloroform

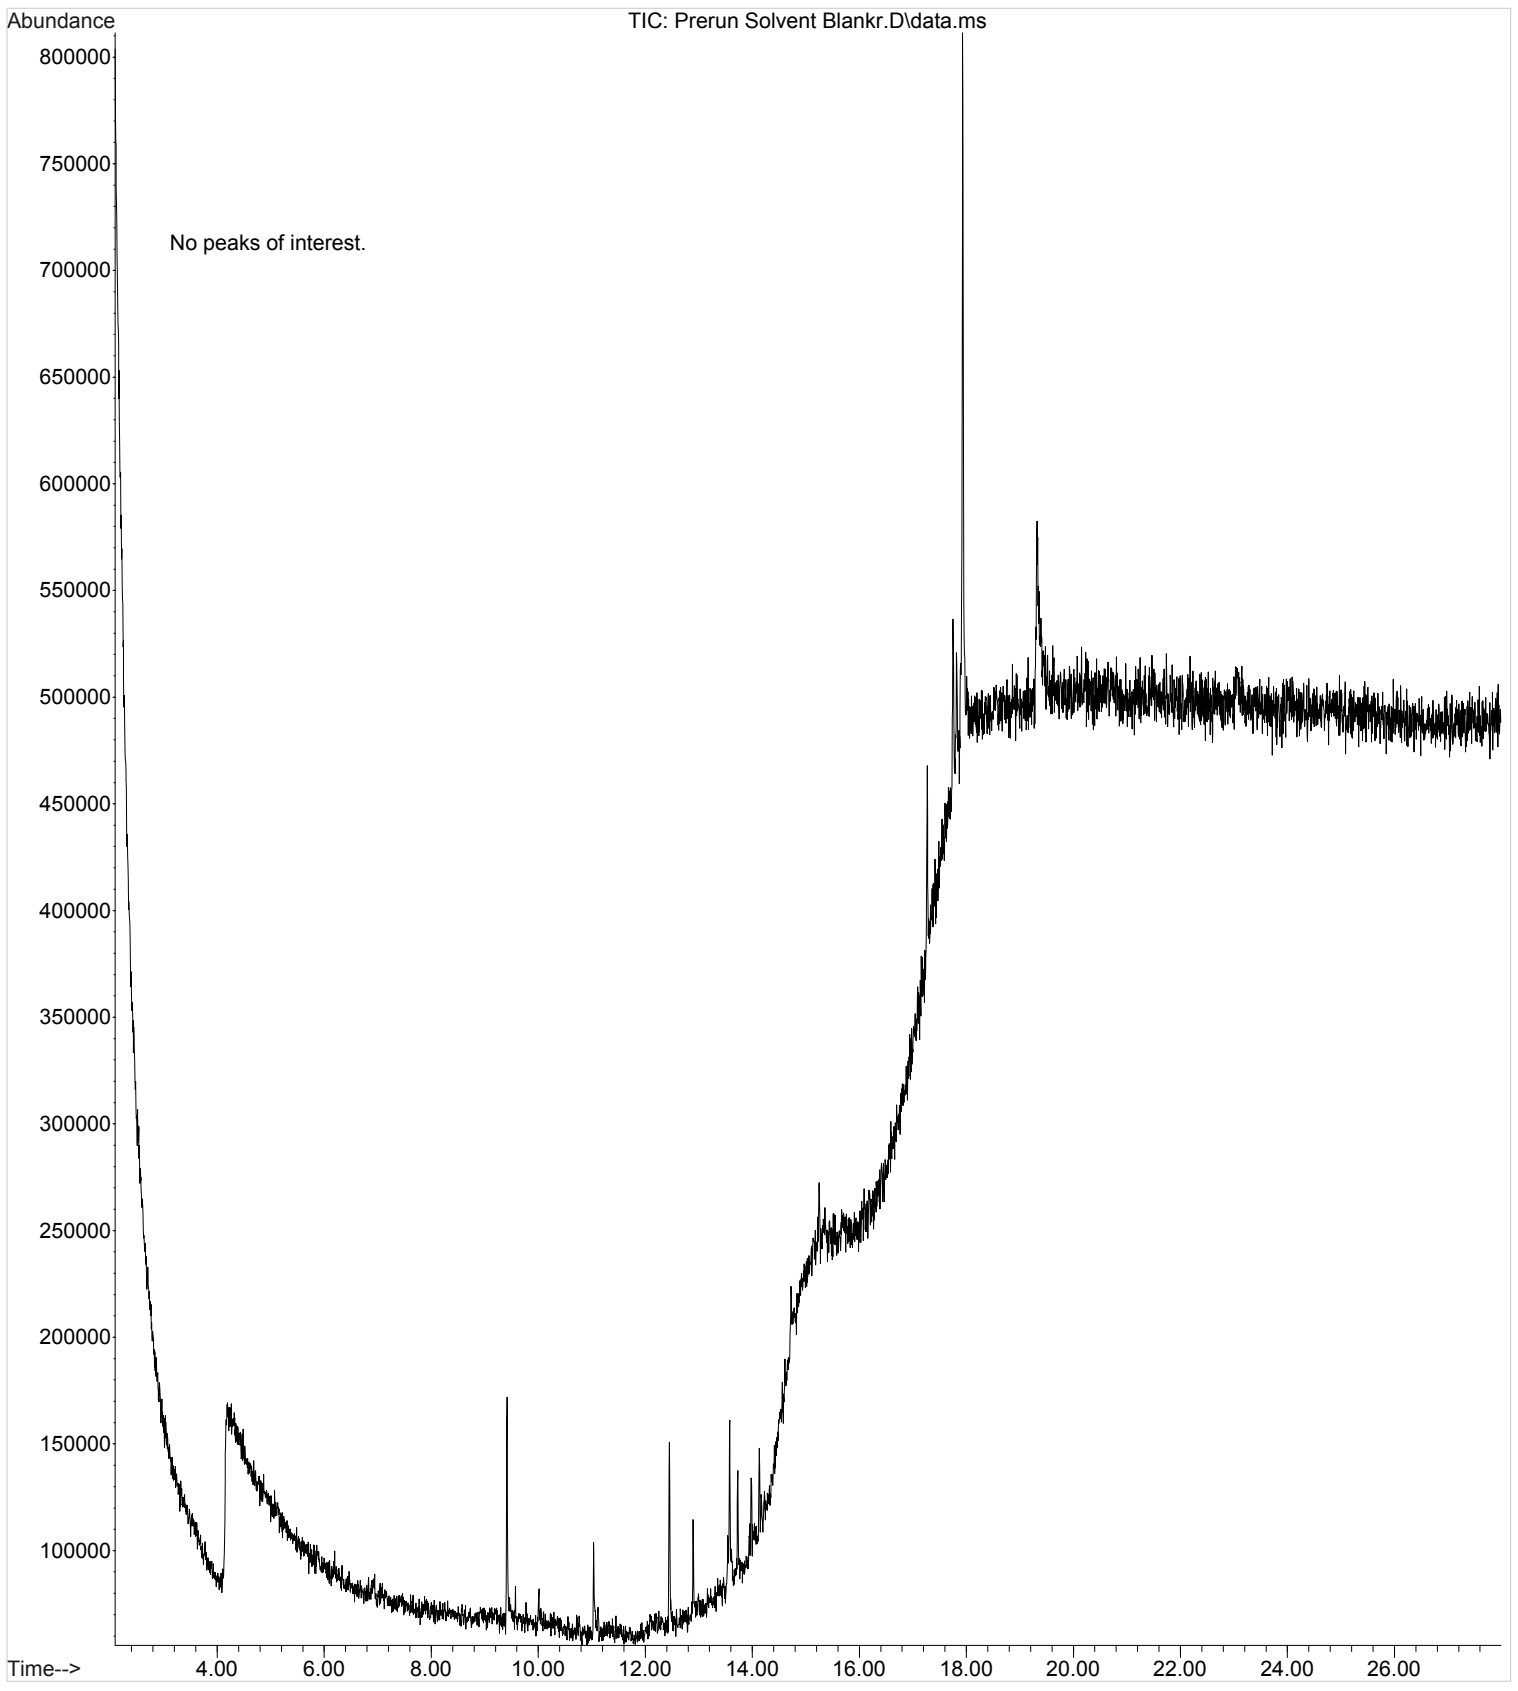



File :I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \prbLK2r.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 19:07 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Solvent Blank
Misc Info : Chloroform

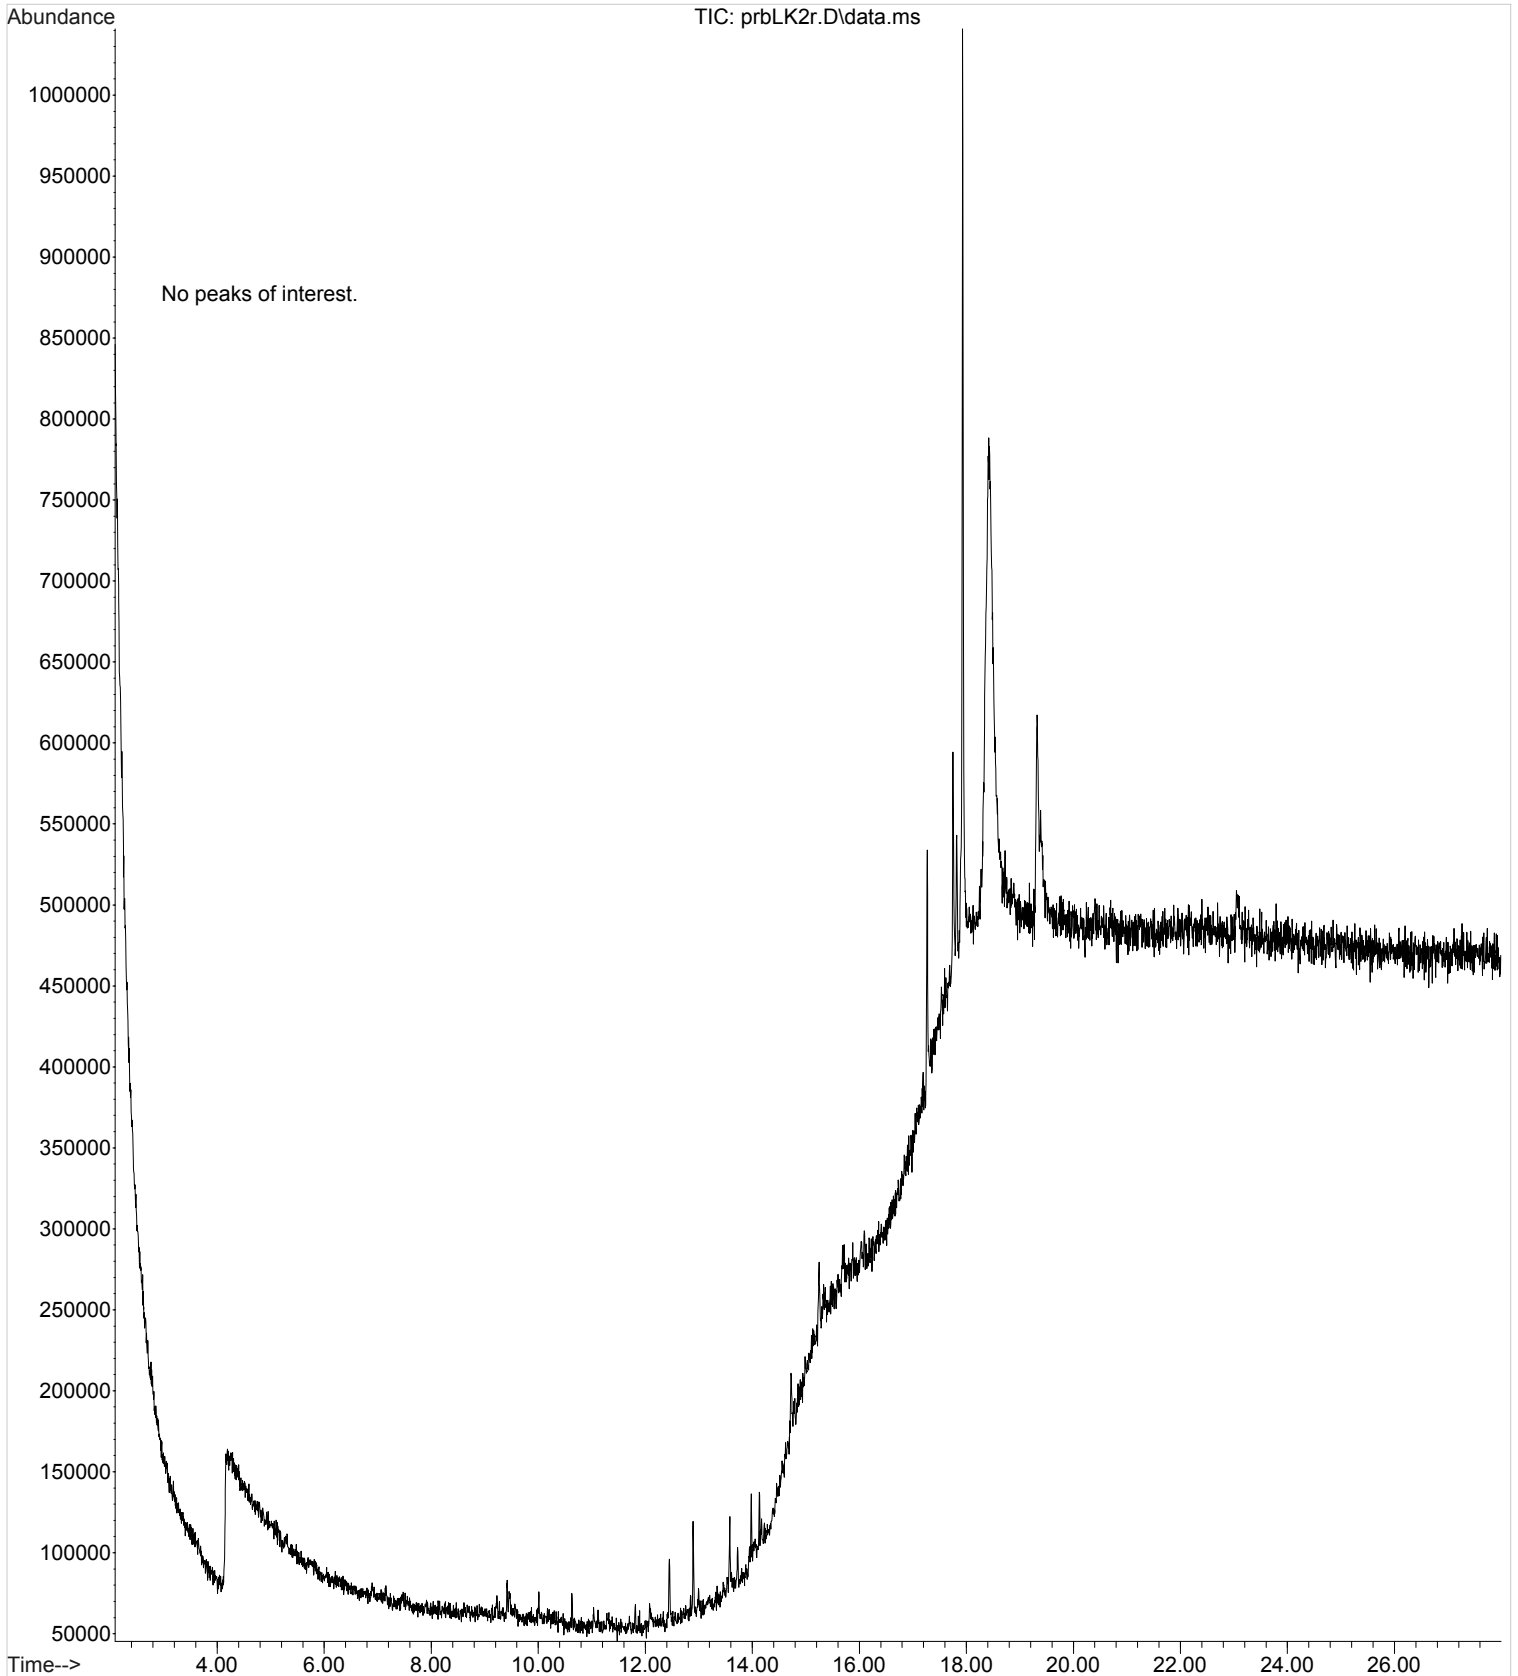



File :I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Negative Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 16:17 using AcqMethod BNSB120510.M
Sample Name: Negative Control - Utak Lot B1013
Misc Info : Analytical Method 3.6.1

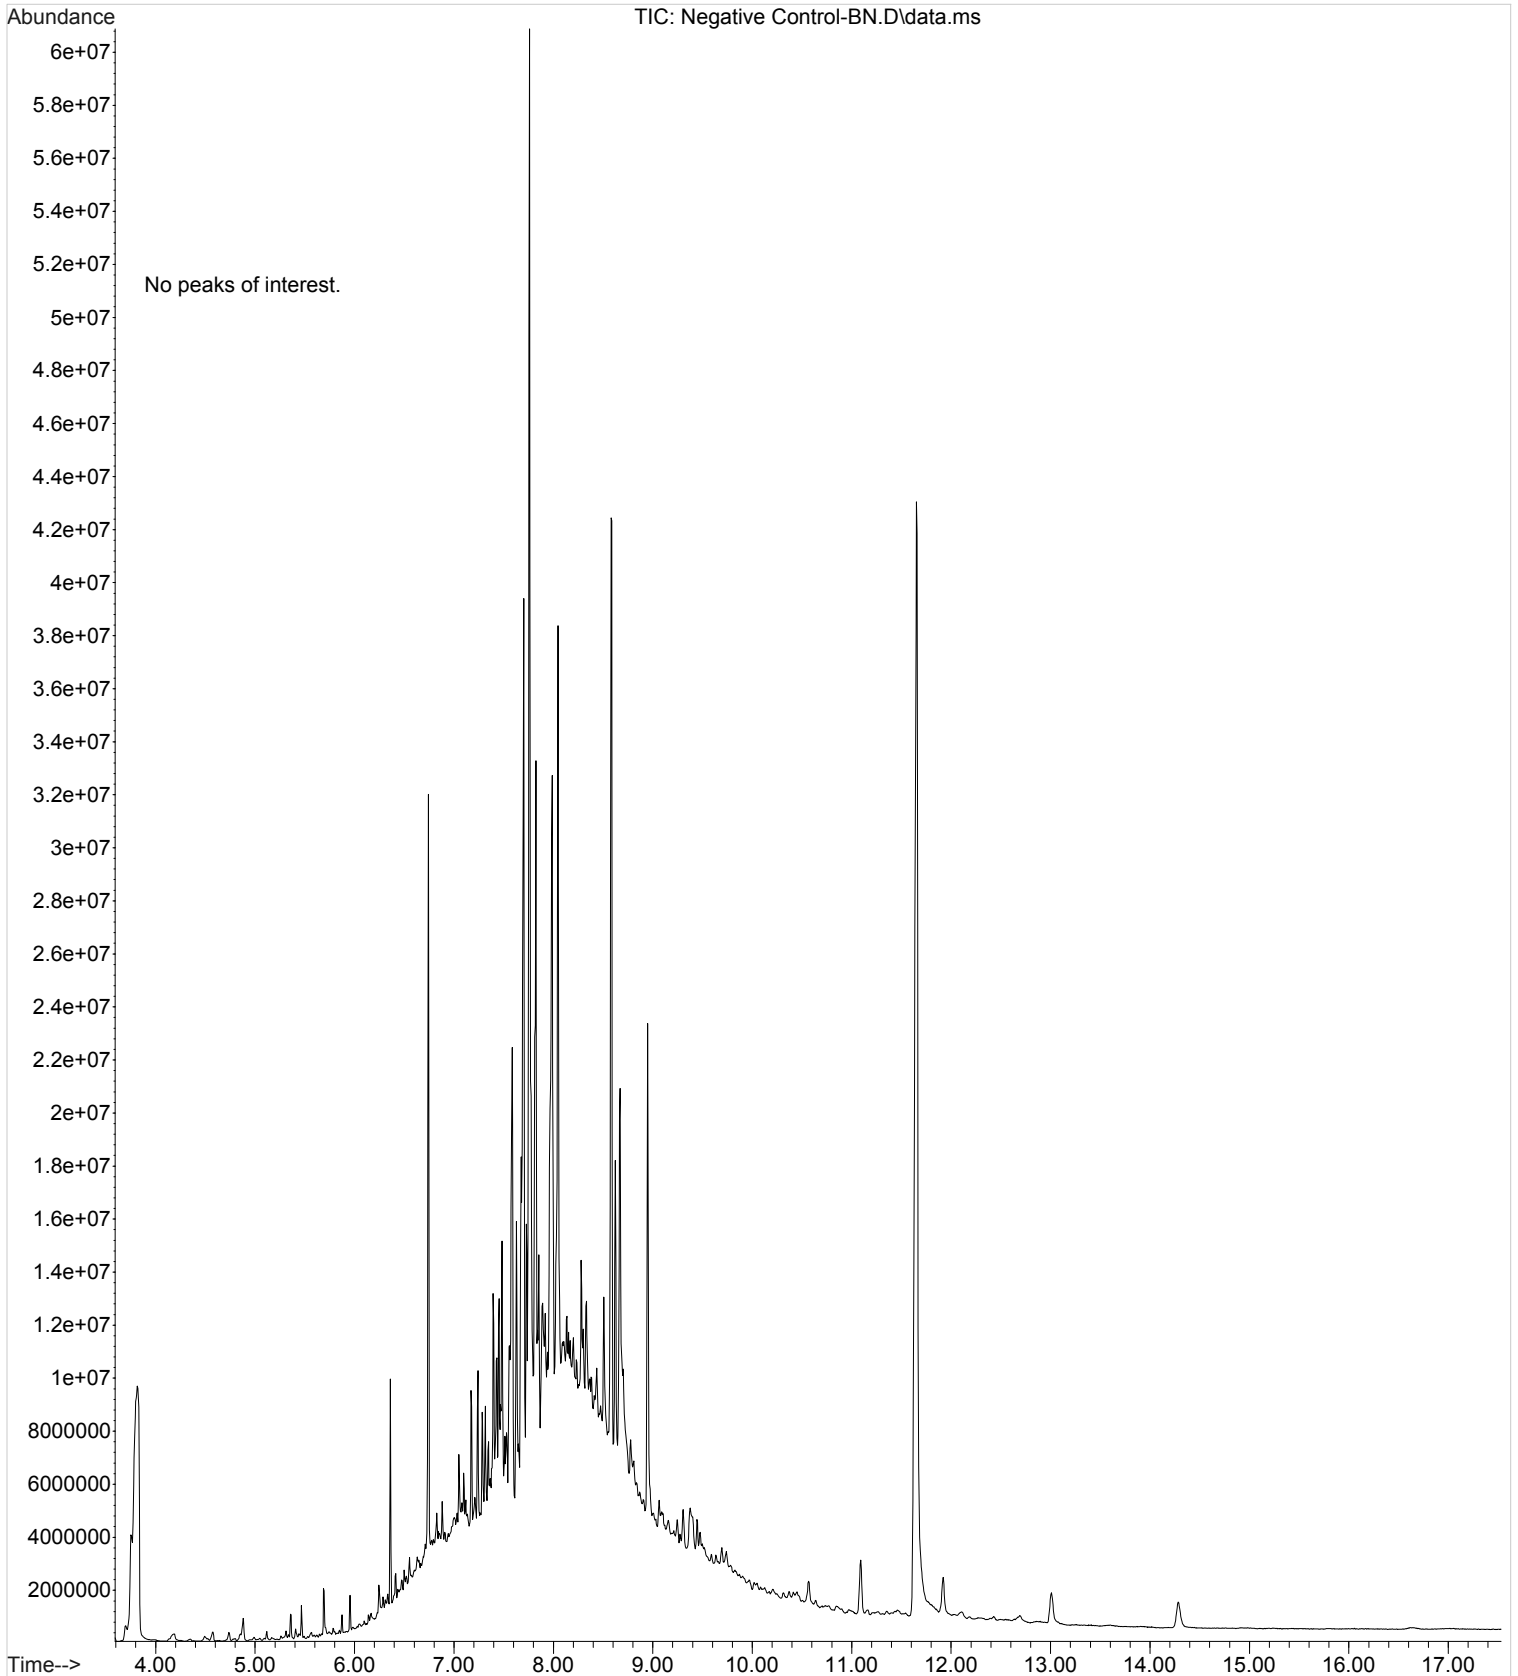



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Negative Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 17:59 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Negative Control - Utak Lot B1013
Misc Info : Analytical Method 3.6.1

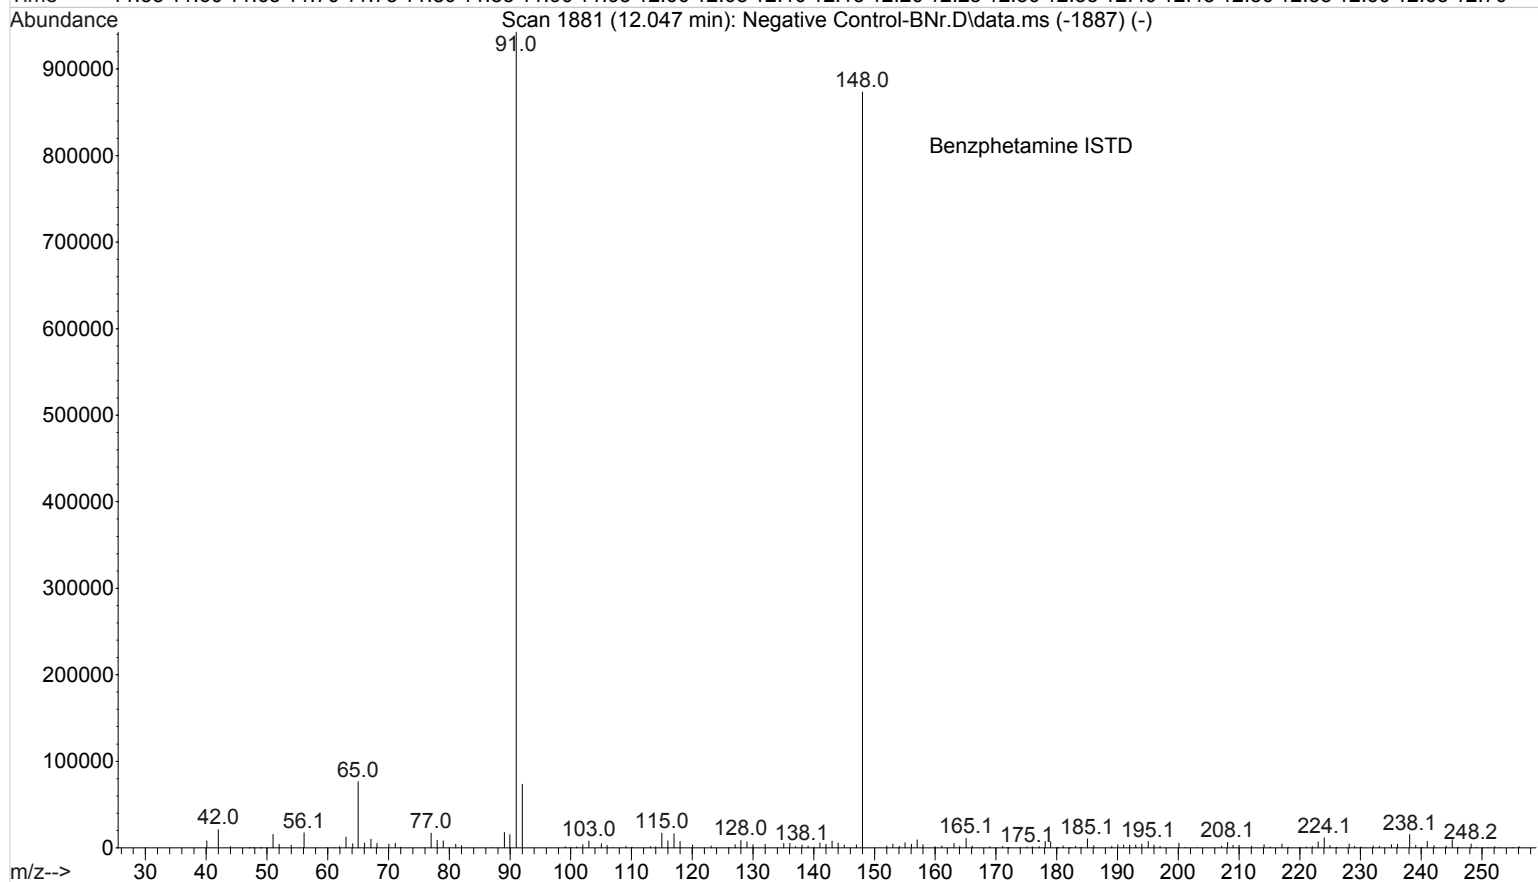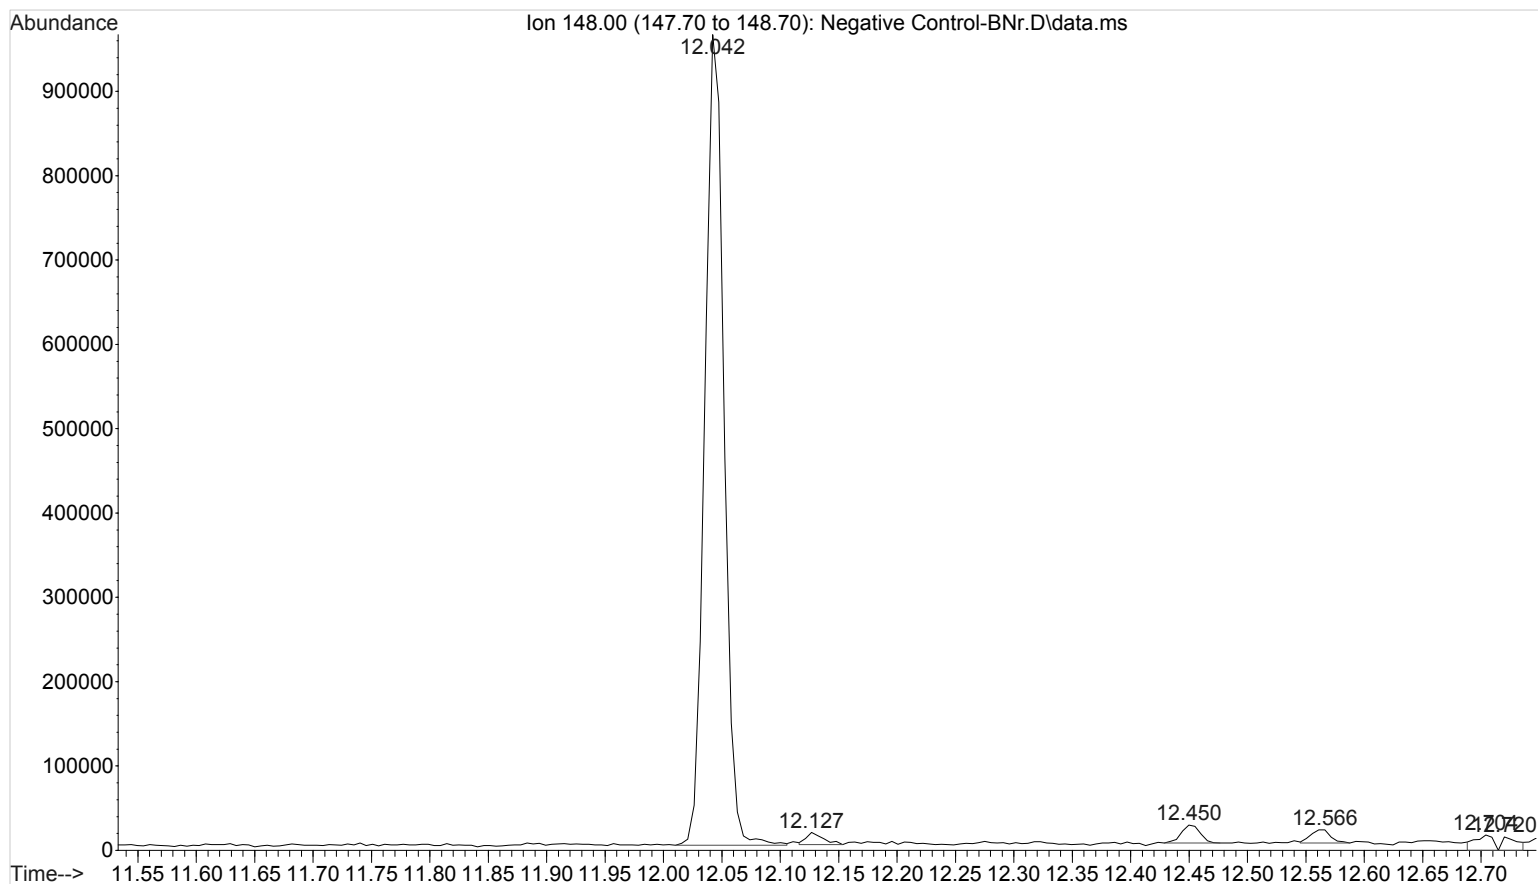



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Negative Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 17:59 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Negative Control - Utak Lot B1013
Misc Info : Analytical Method 3.6.1

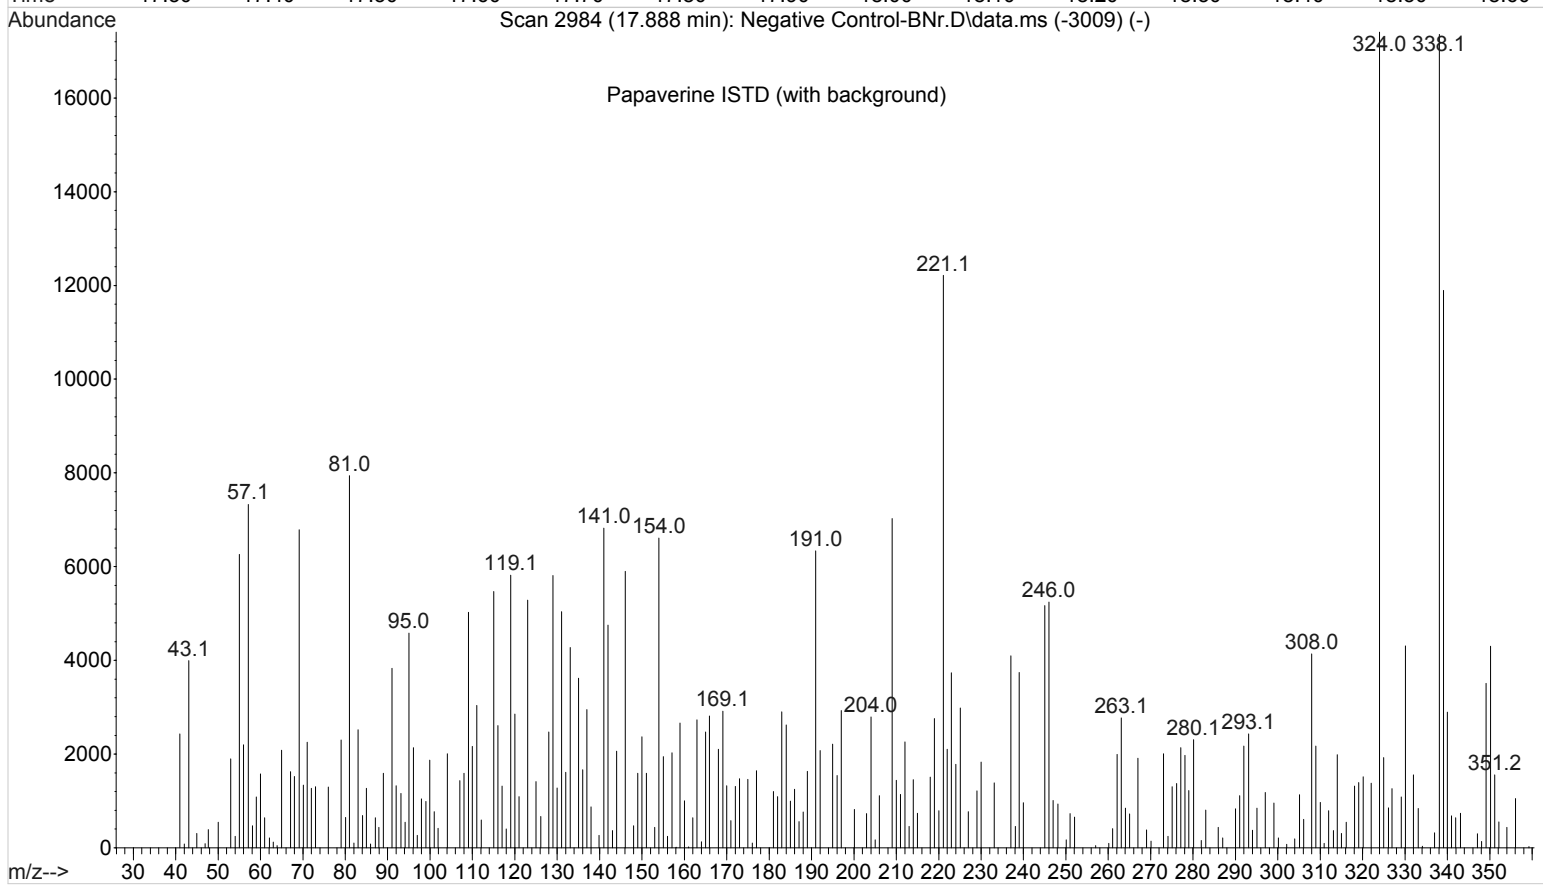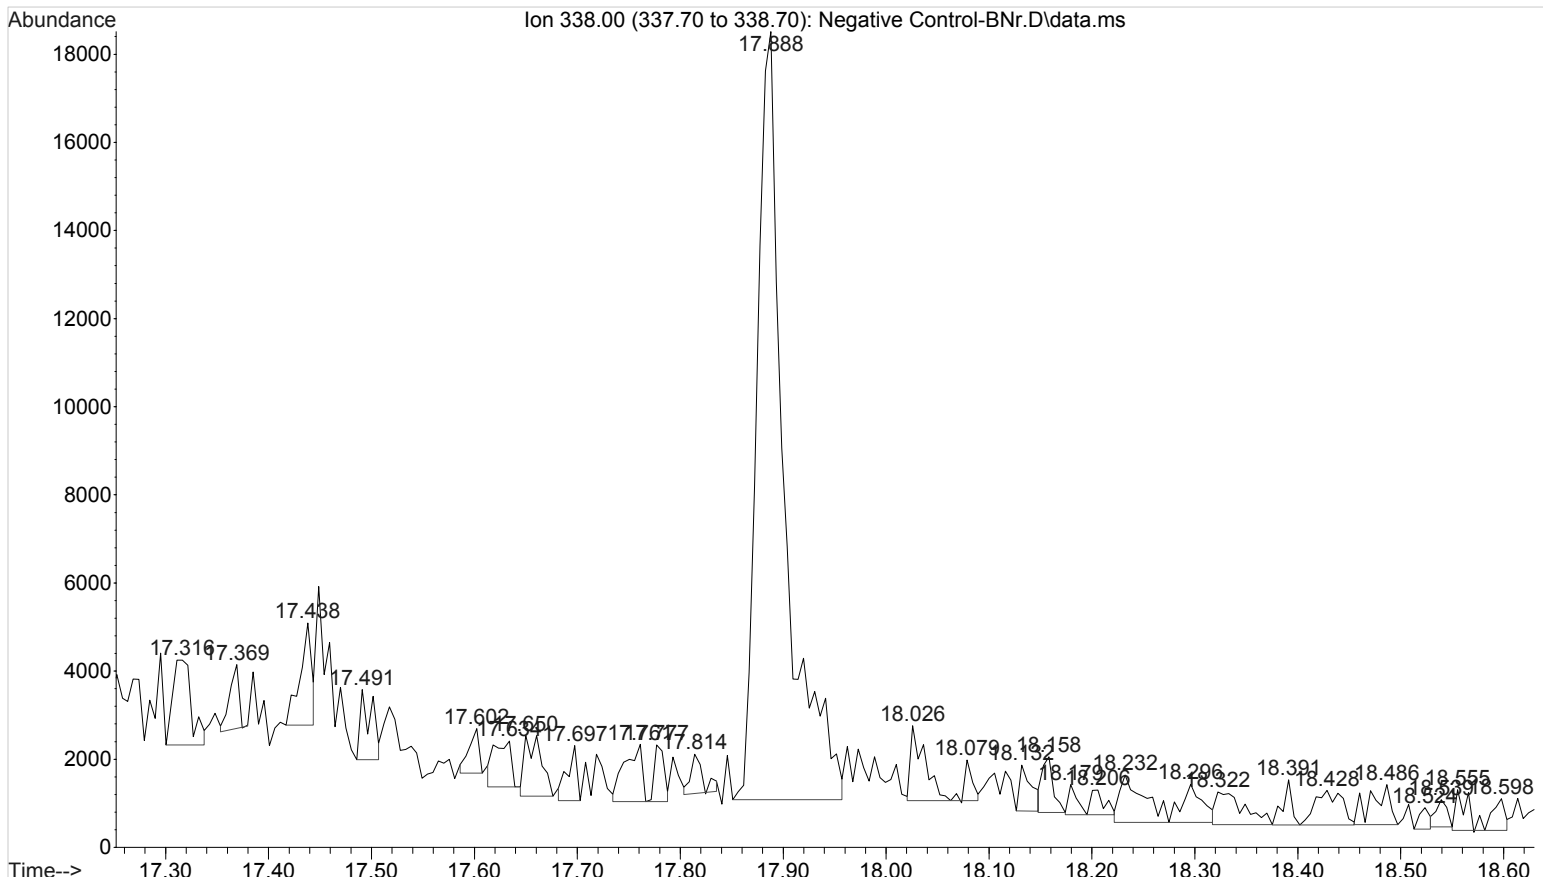

File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Spiked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 18:33 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

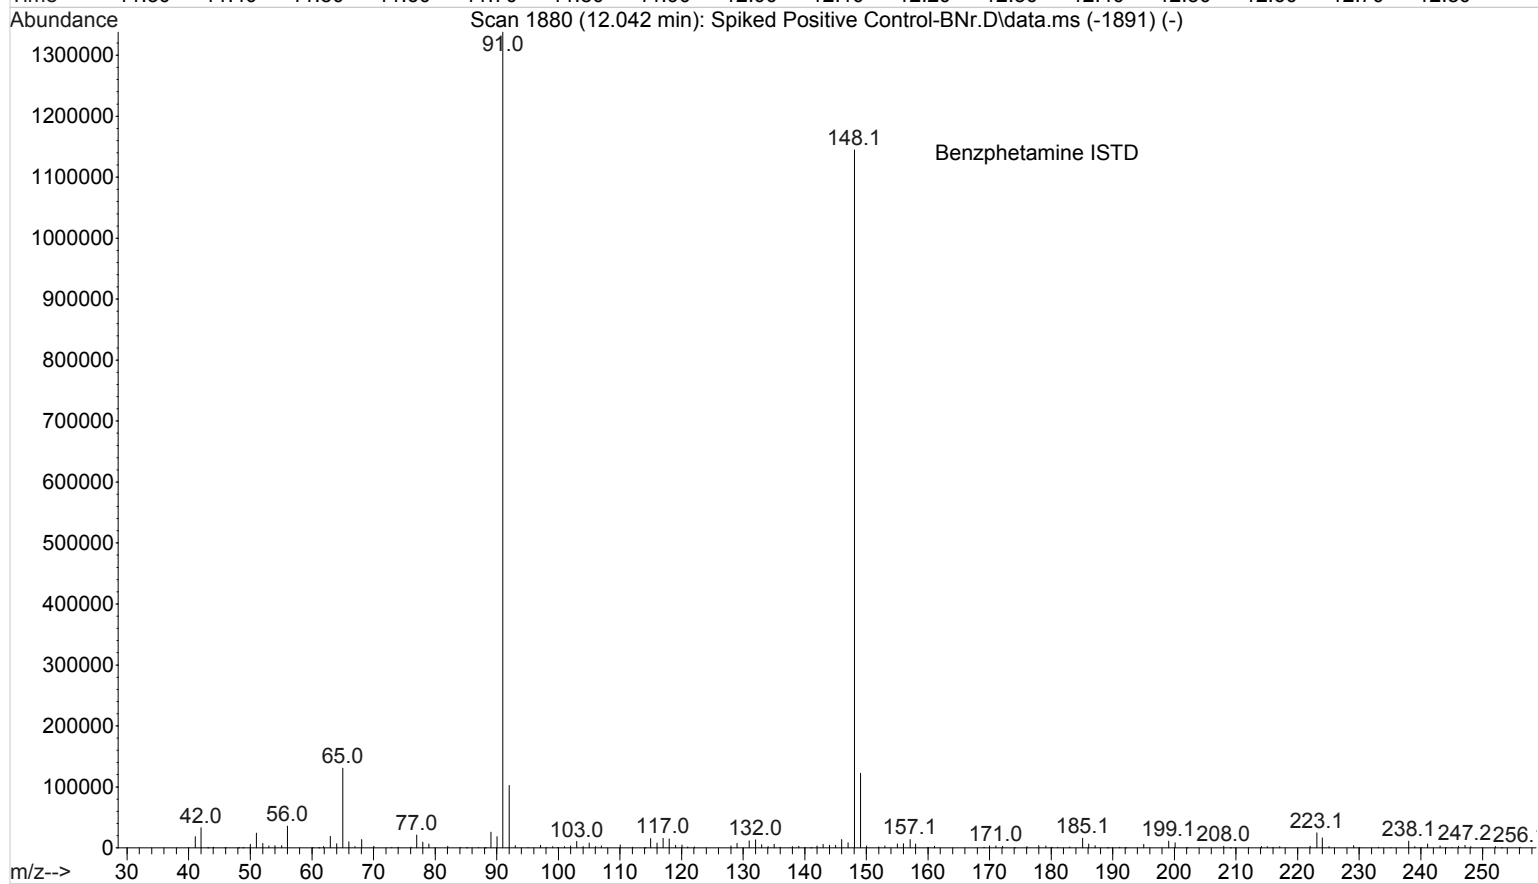
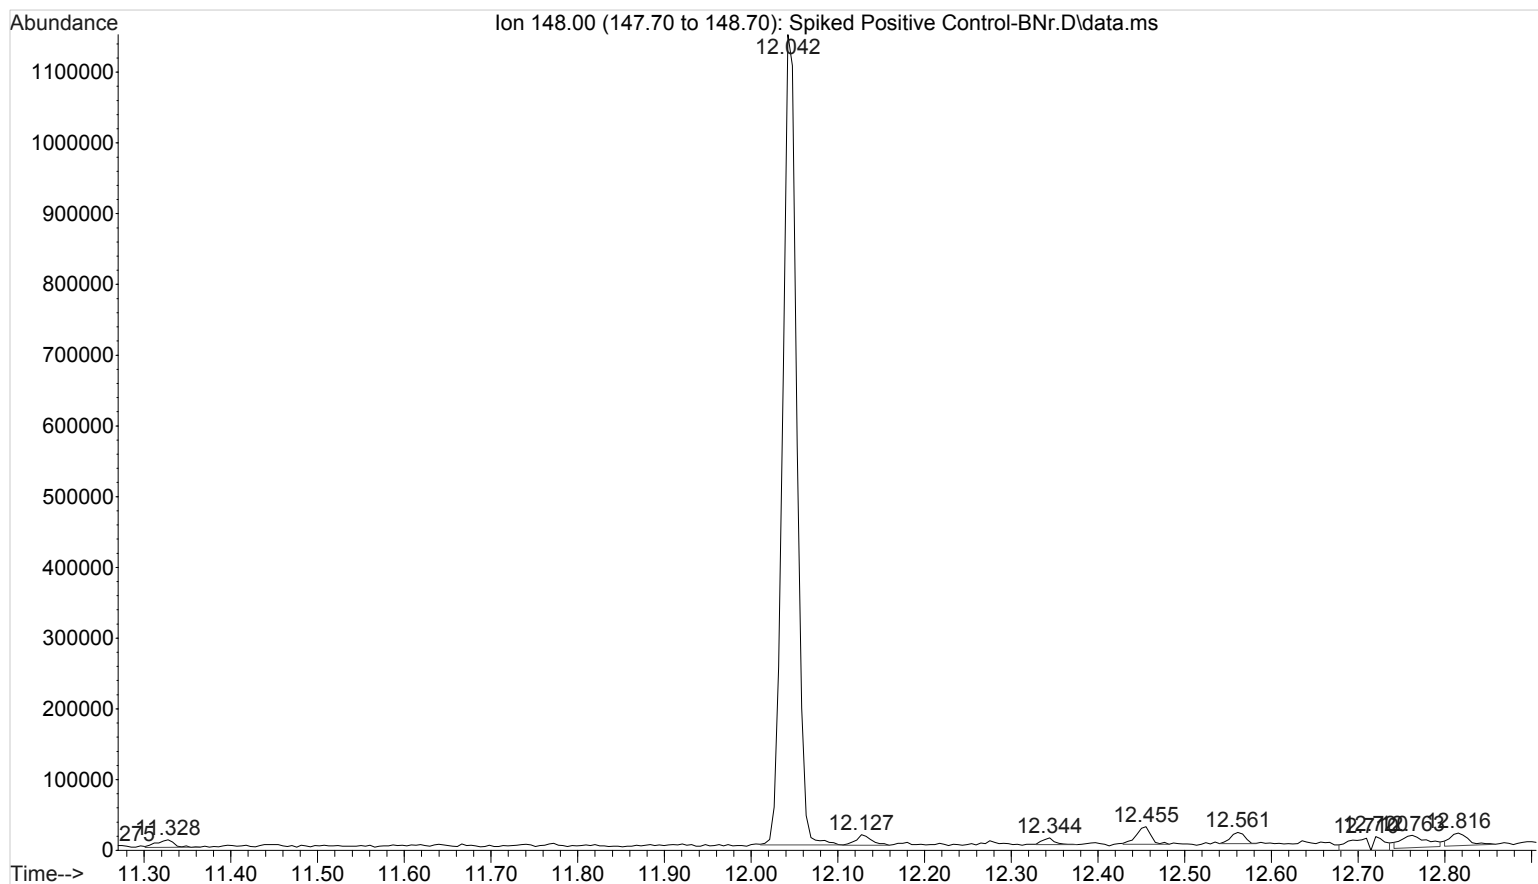


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Spiked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 18:33 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

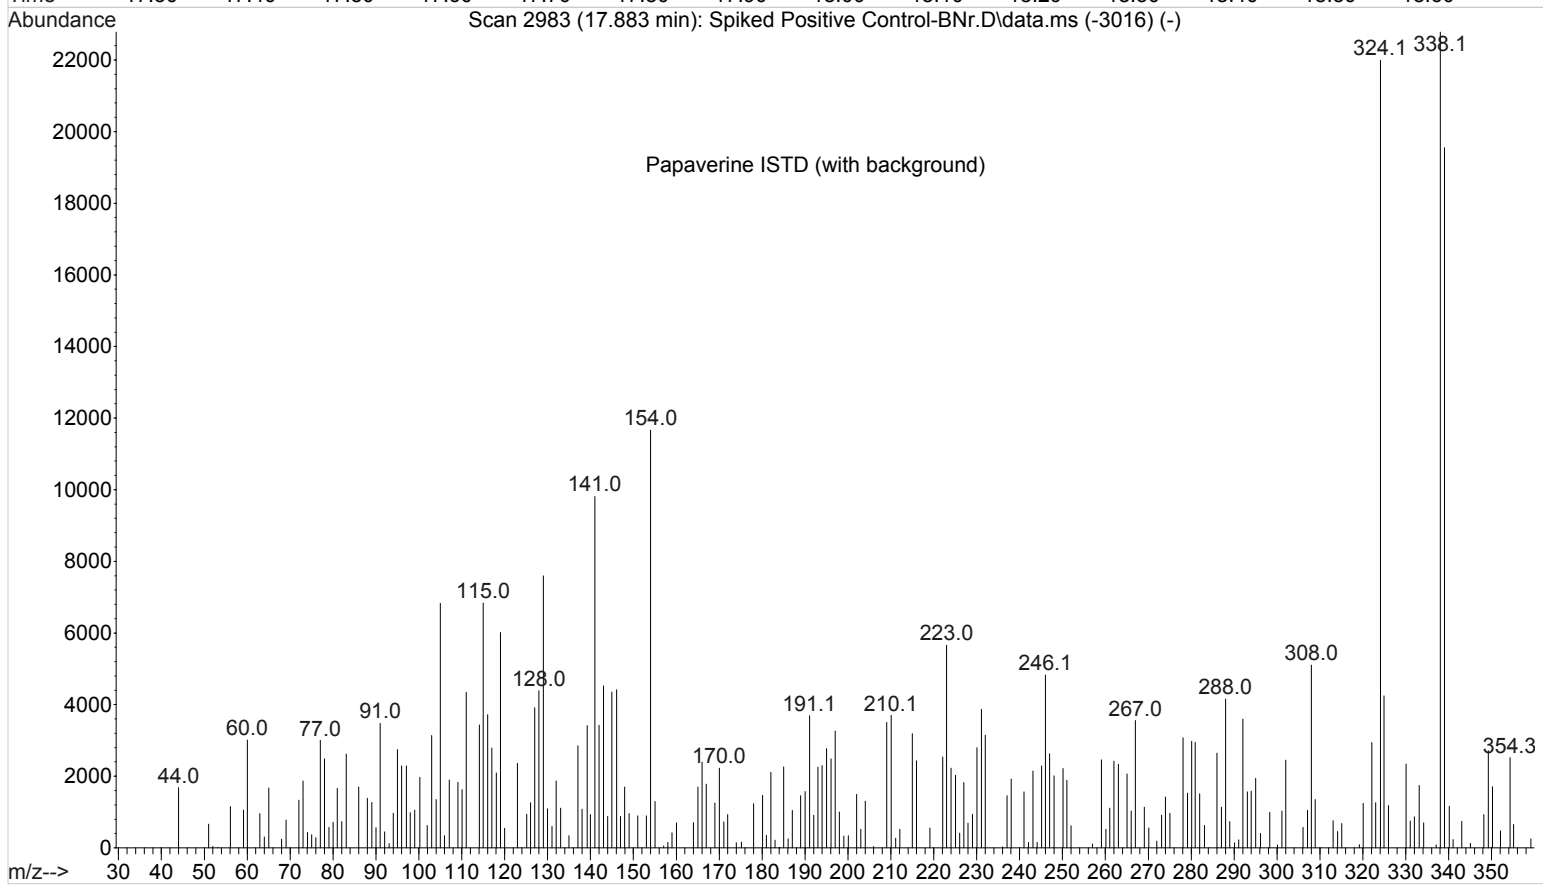
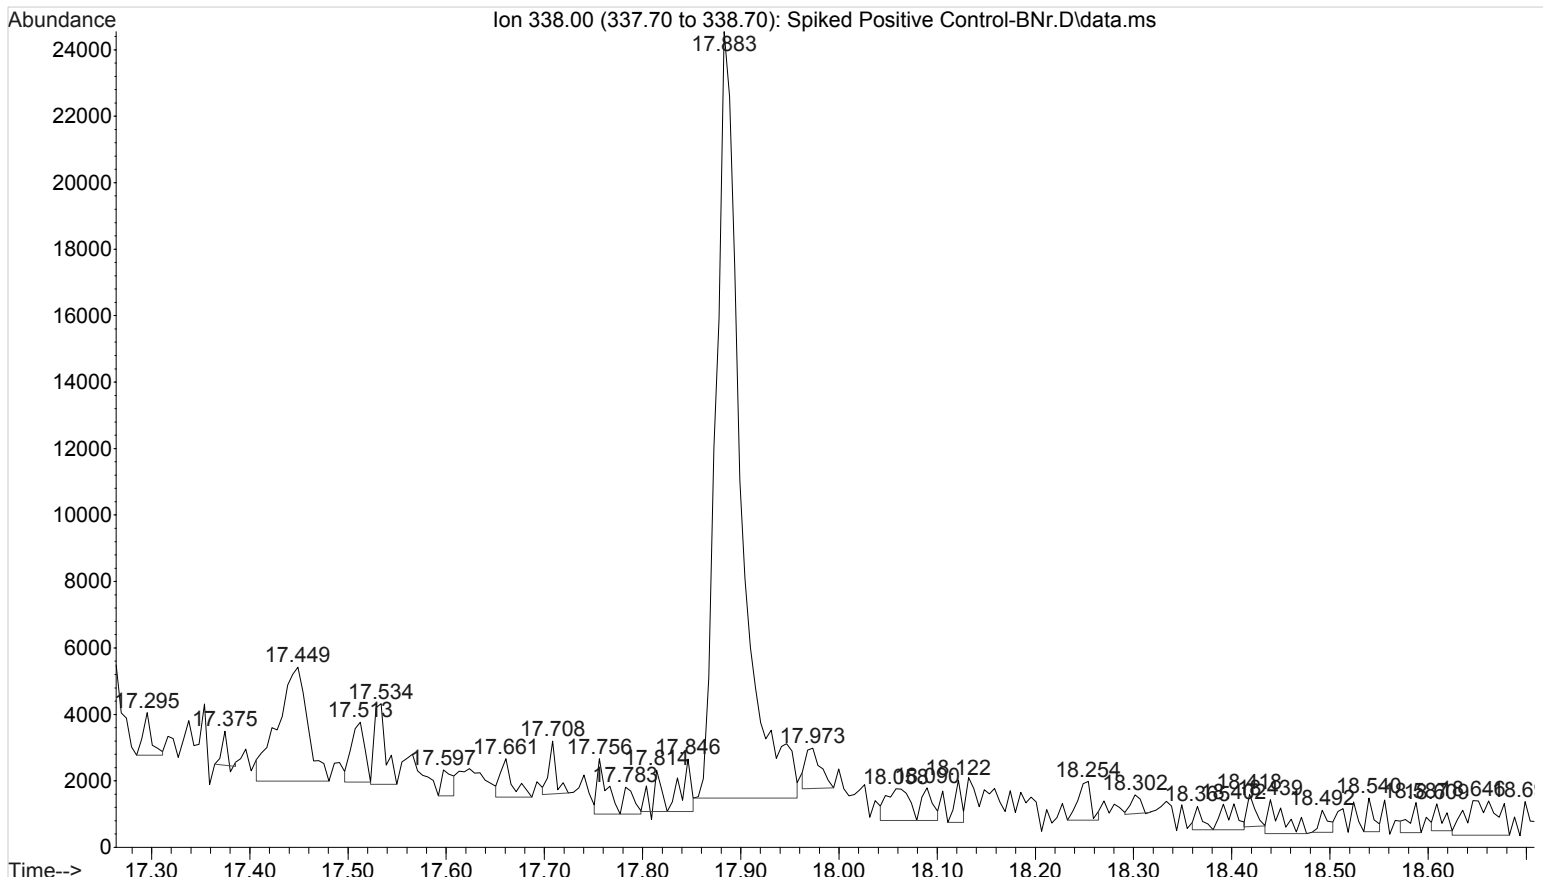


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Spiked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 18:33 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215



CS

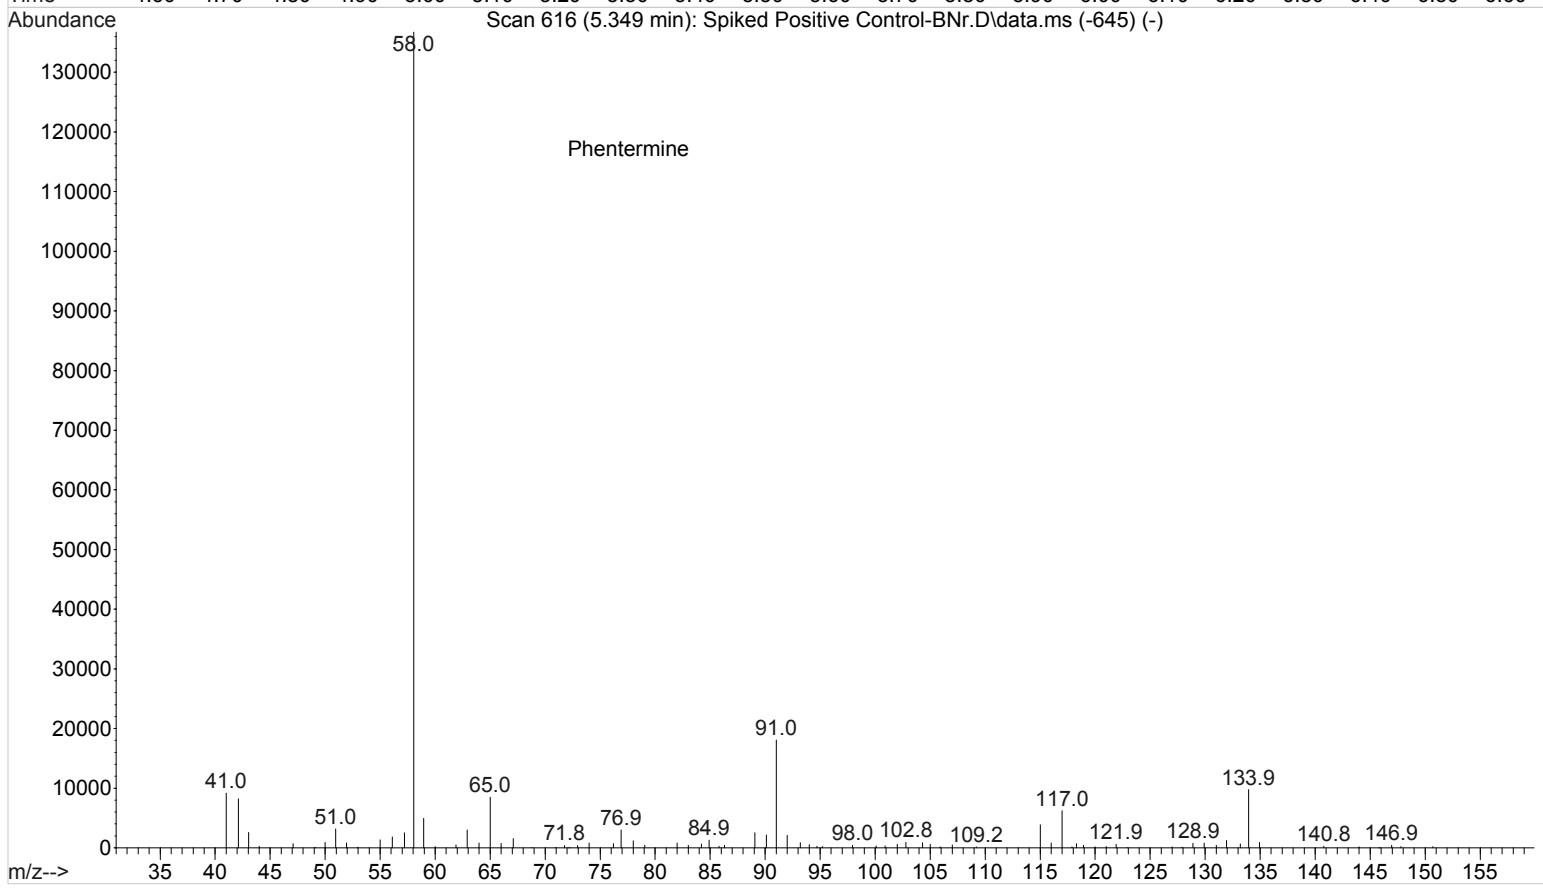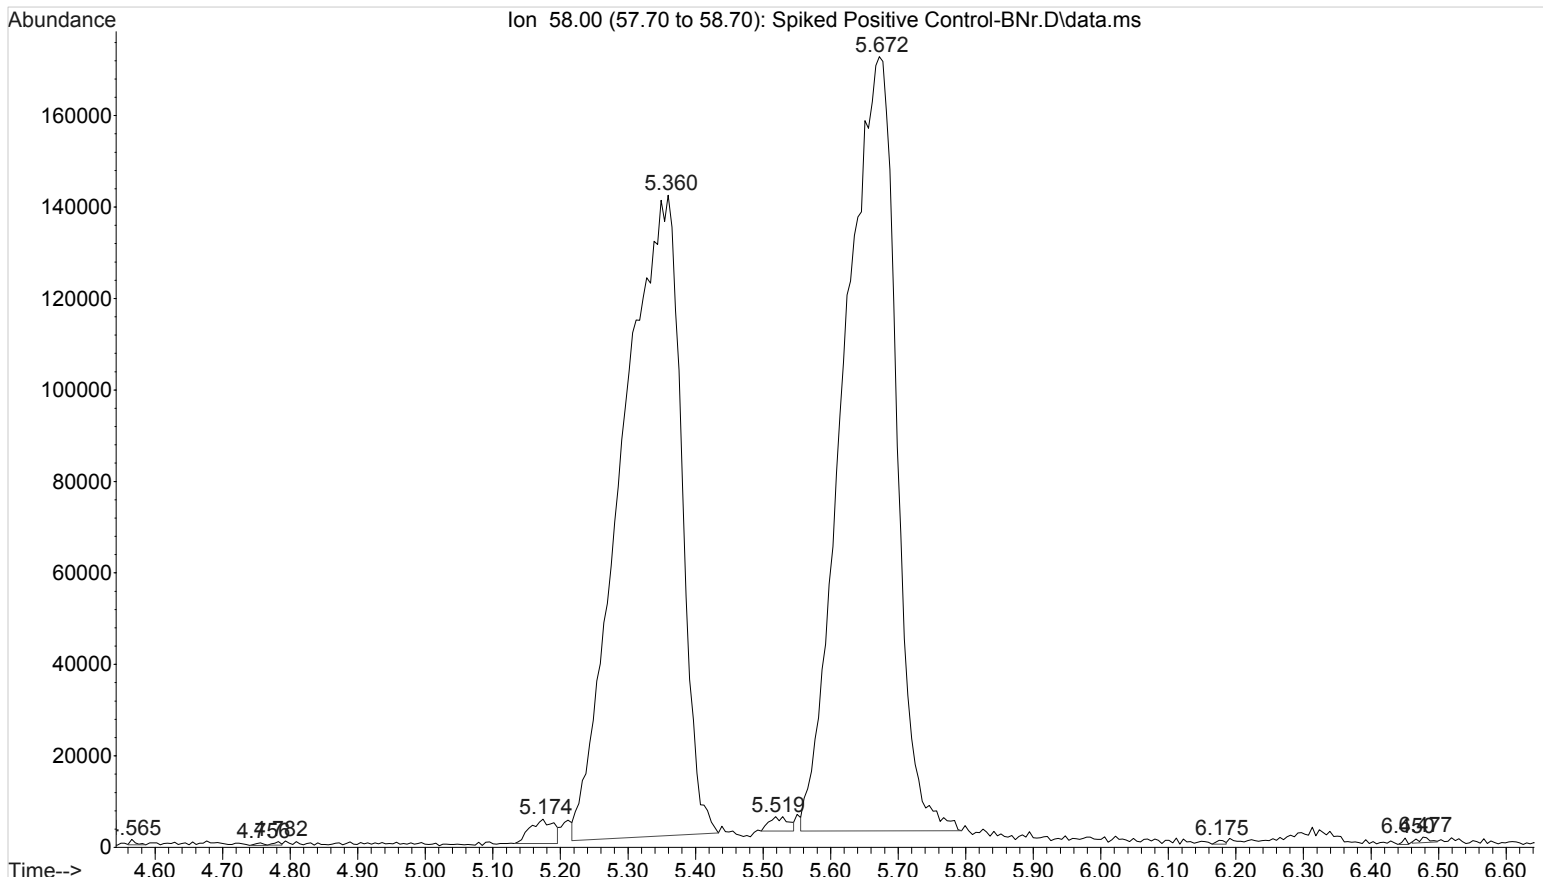

File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Spiked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 18:33 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

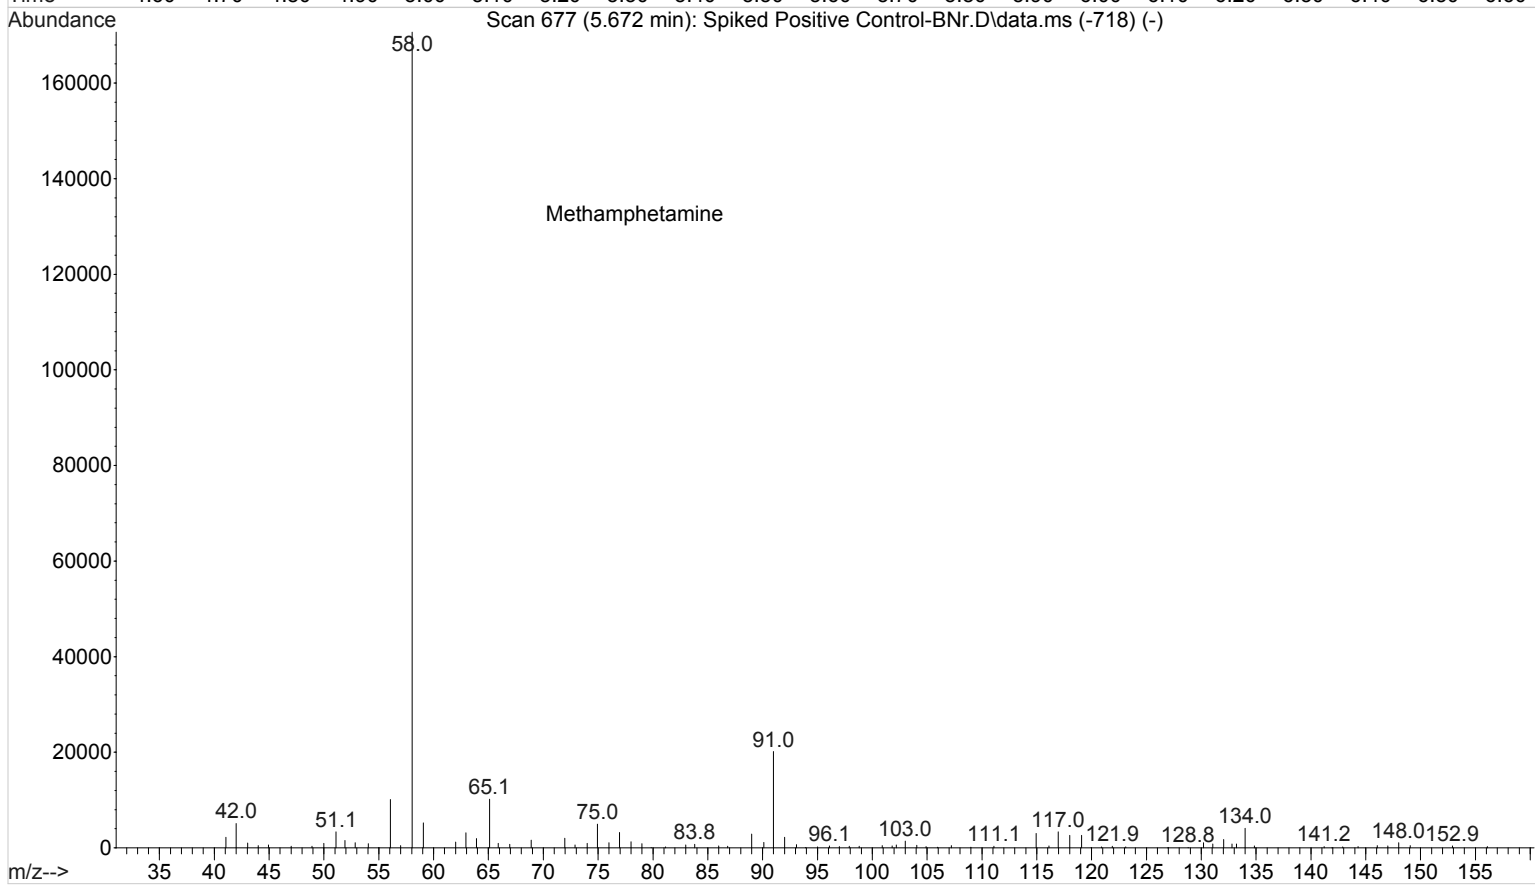
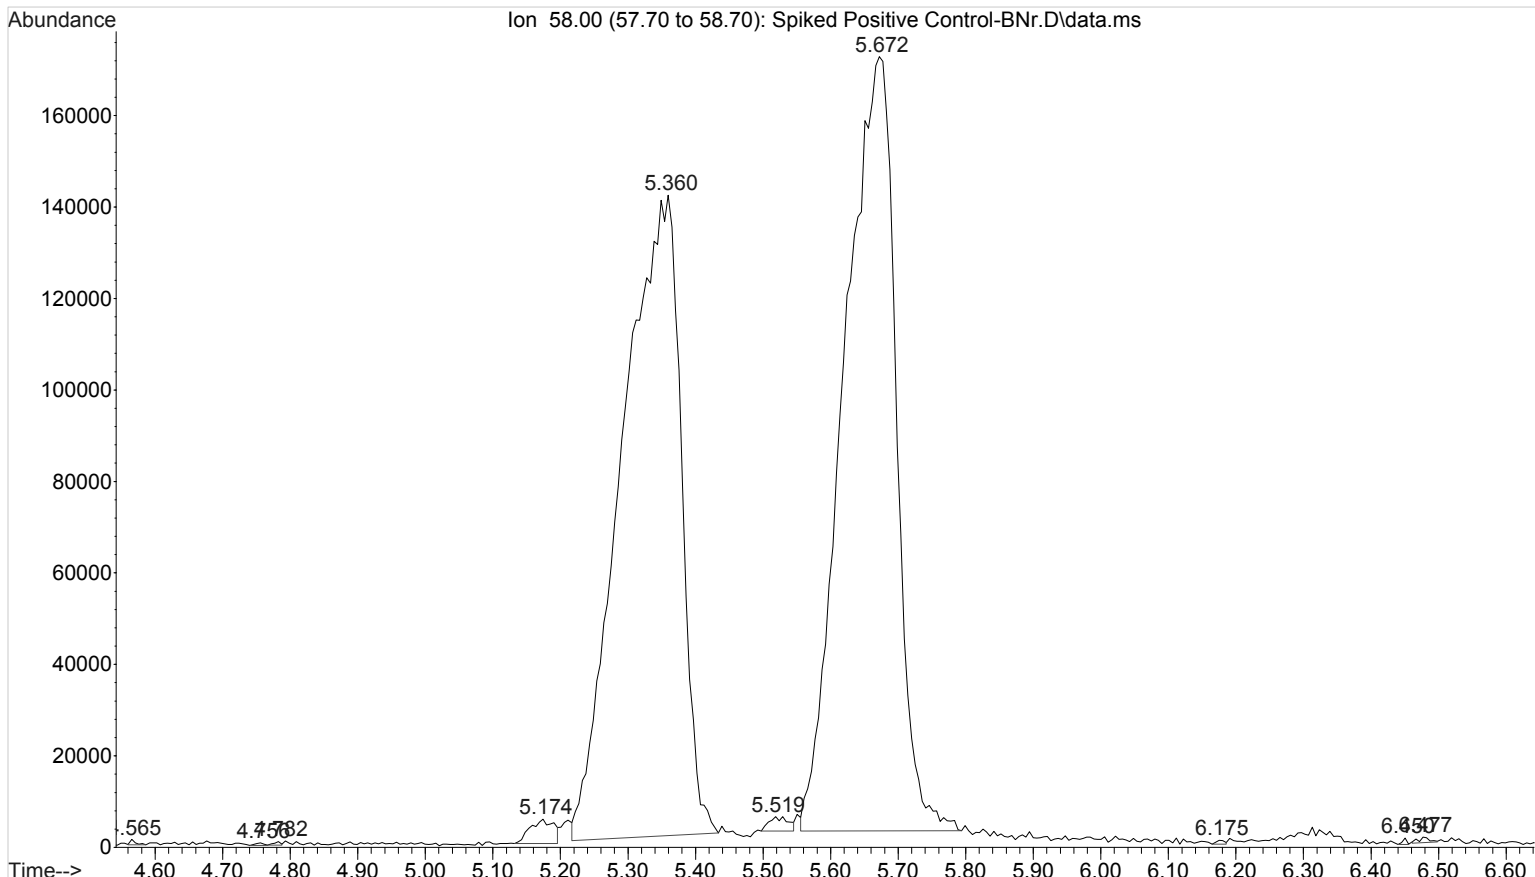


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Spiked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 18:33 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

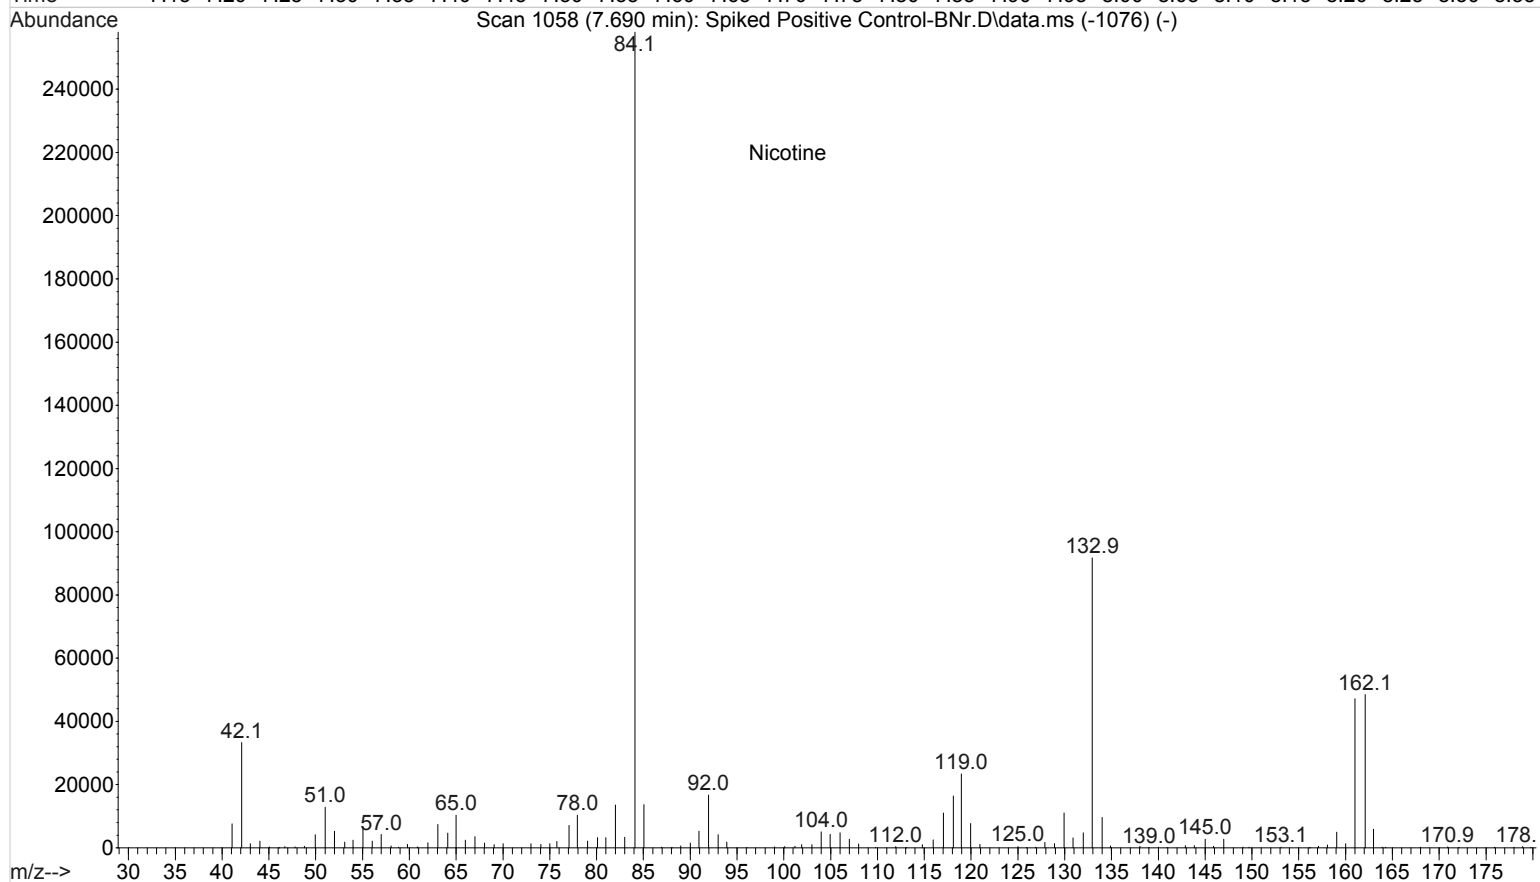
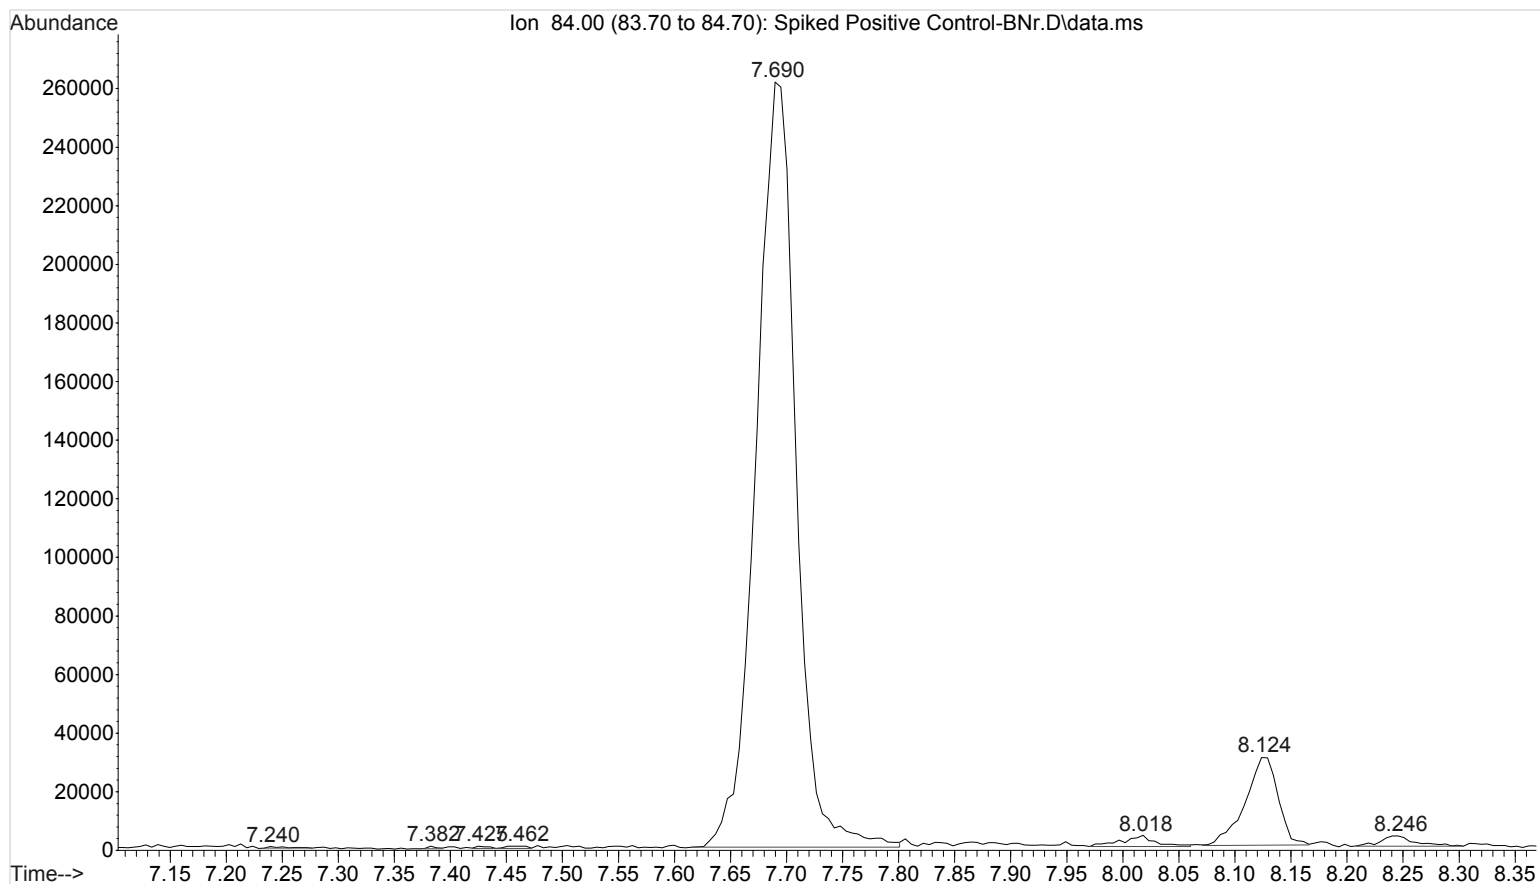


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Spiked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 18:33 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

66

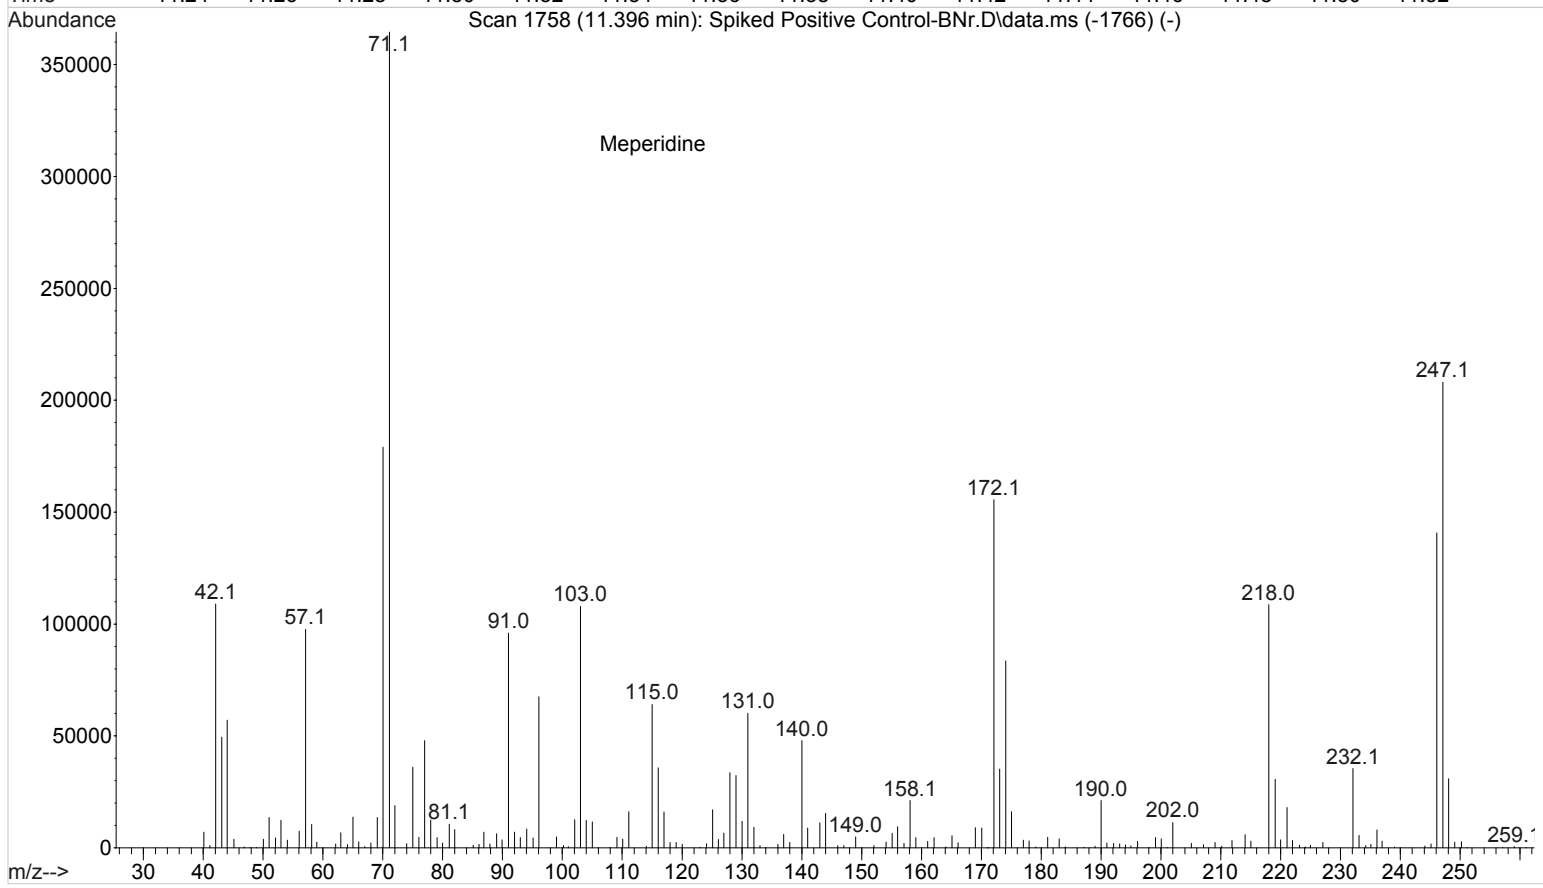
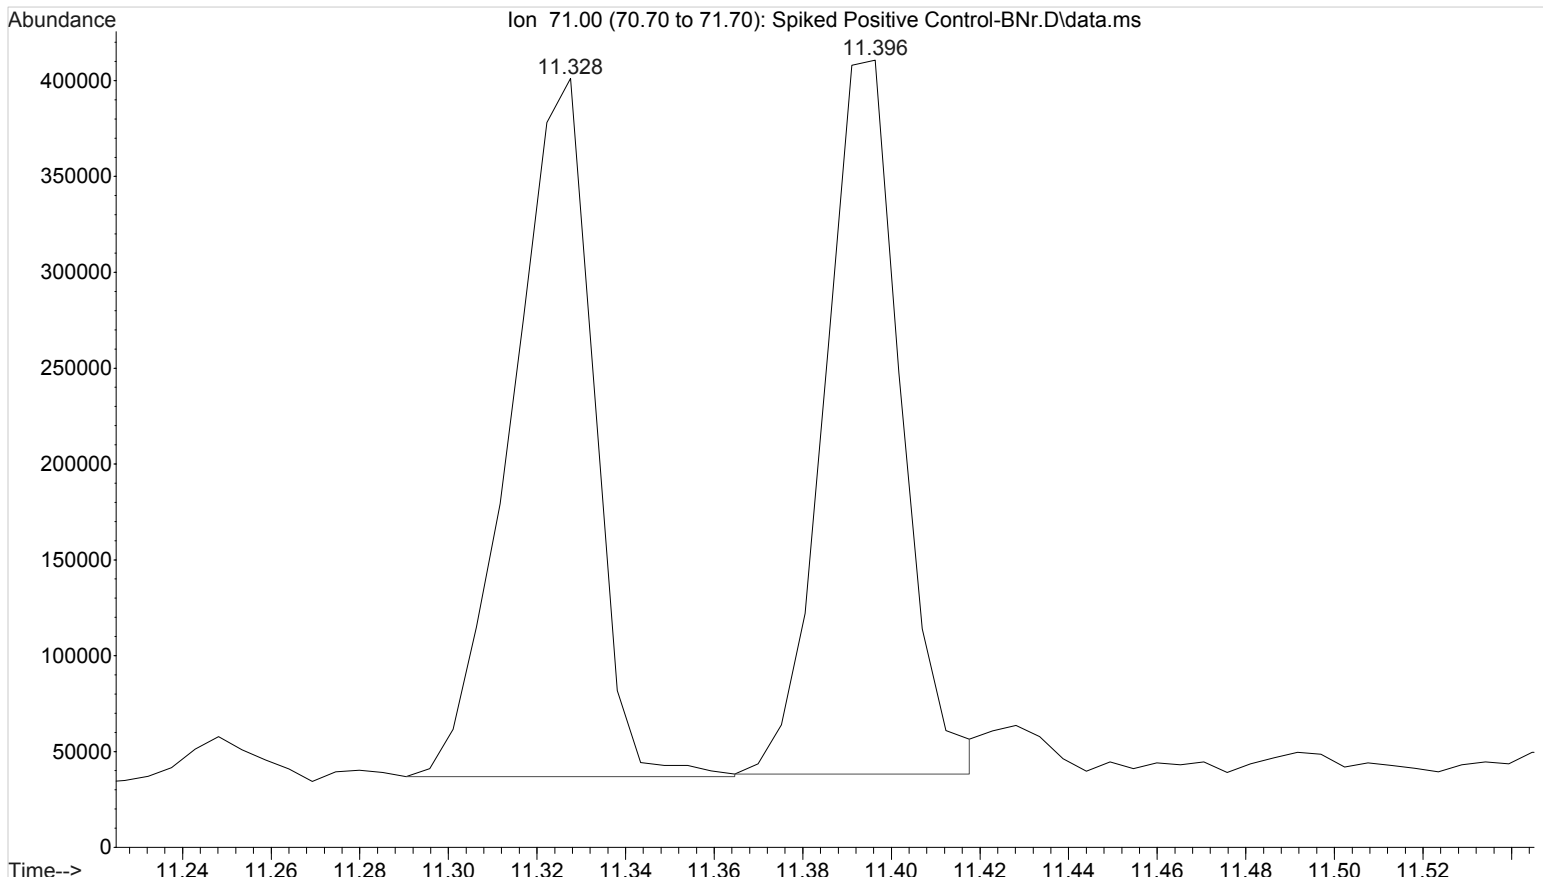


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Spiked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 18:33 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

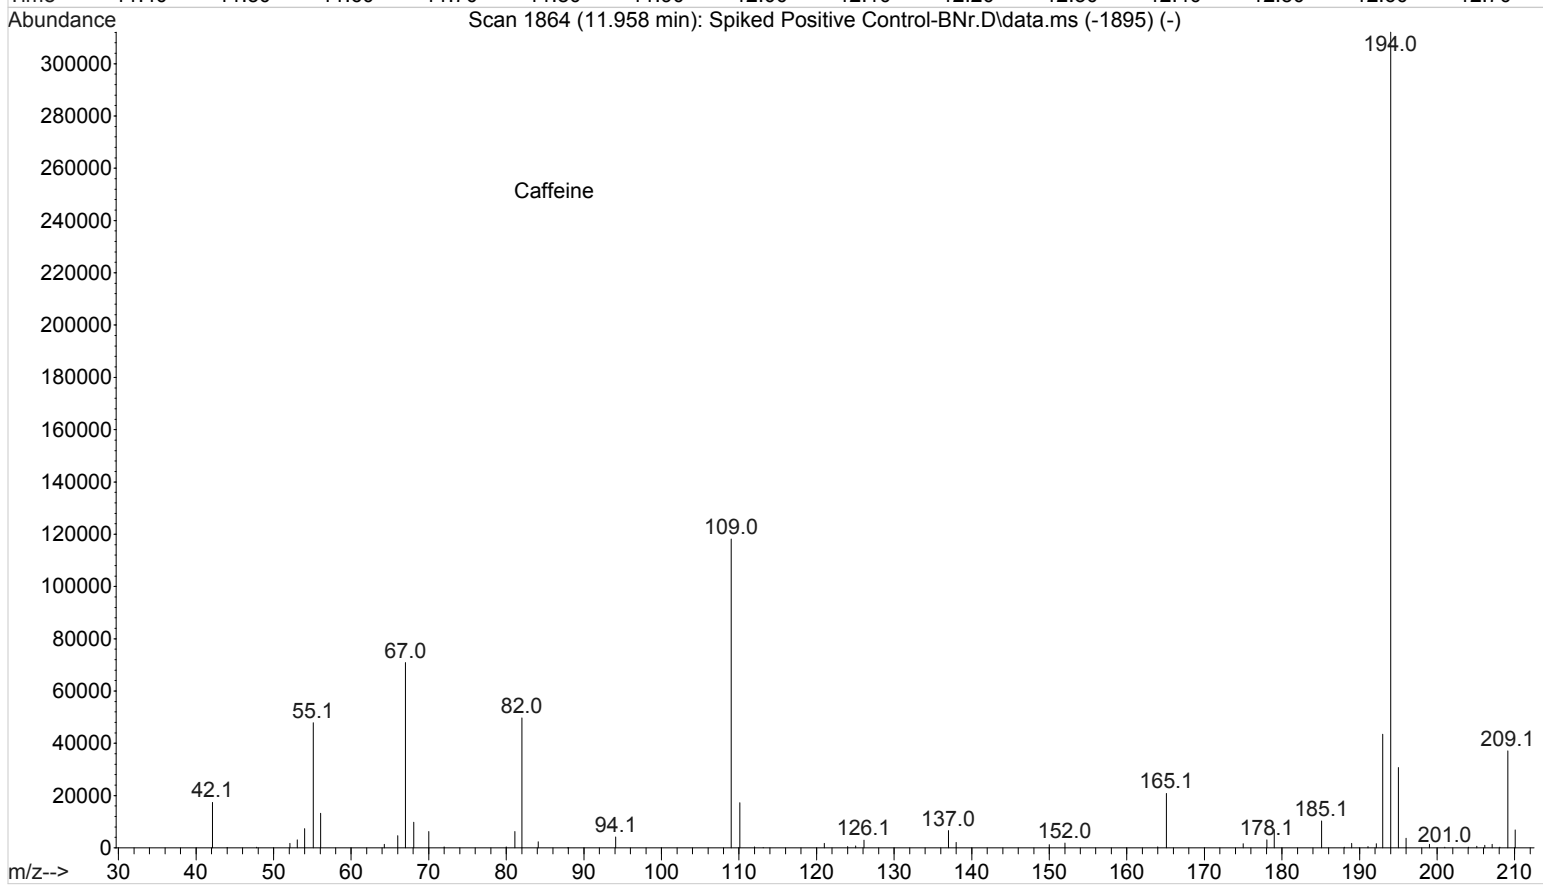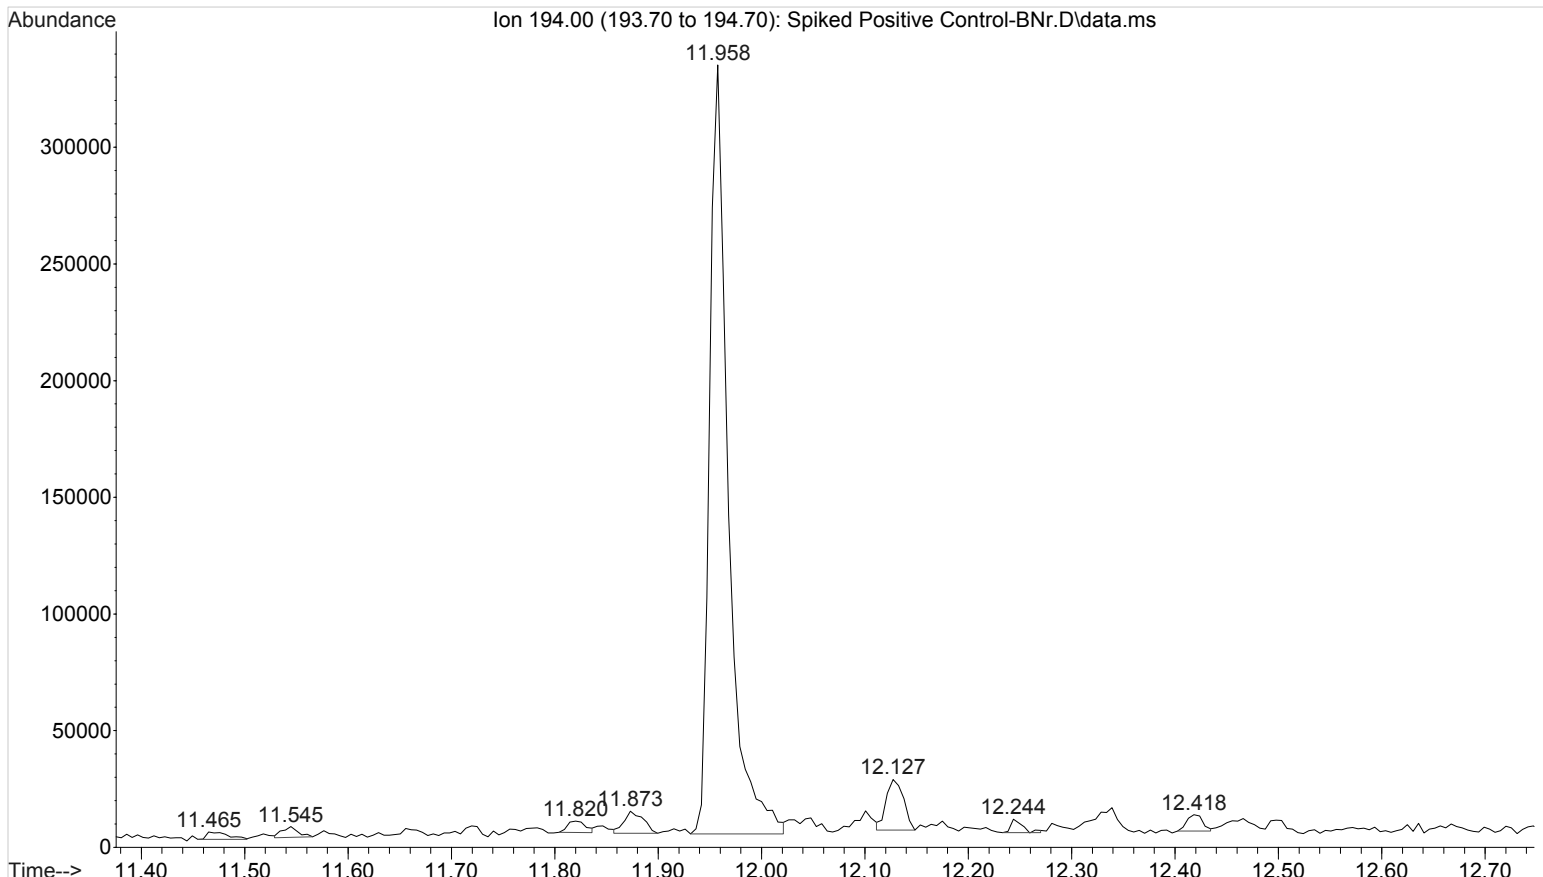



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Spiked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 18:33 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

9

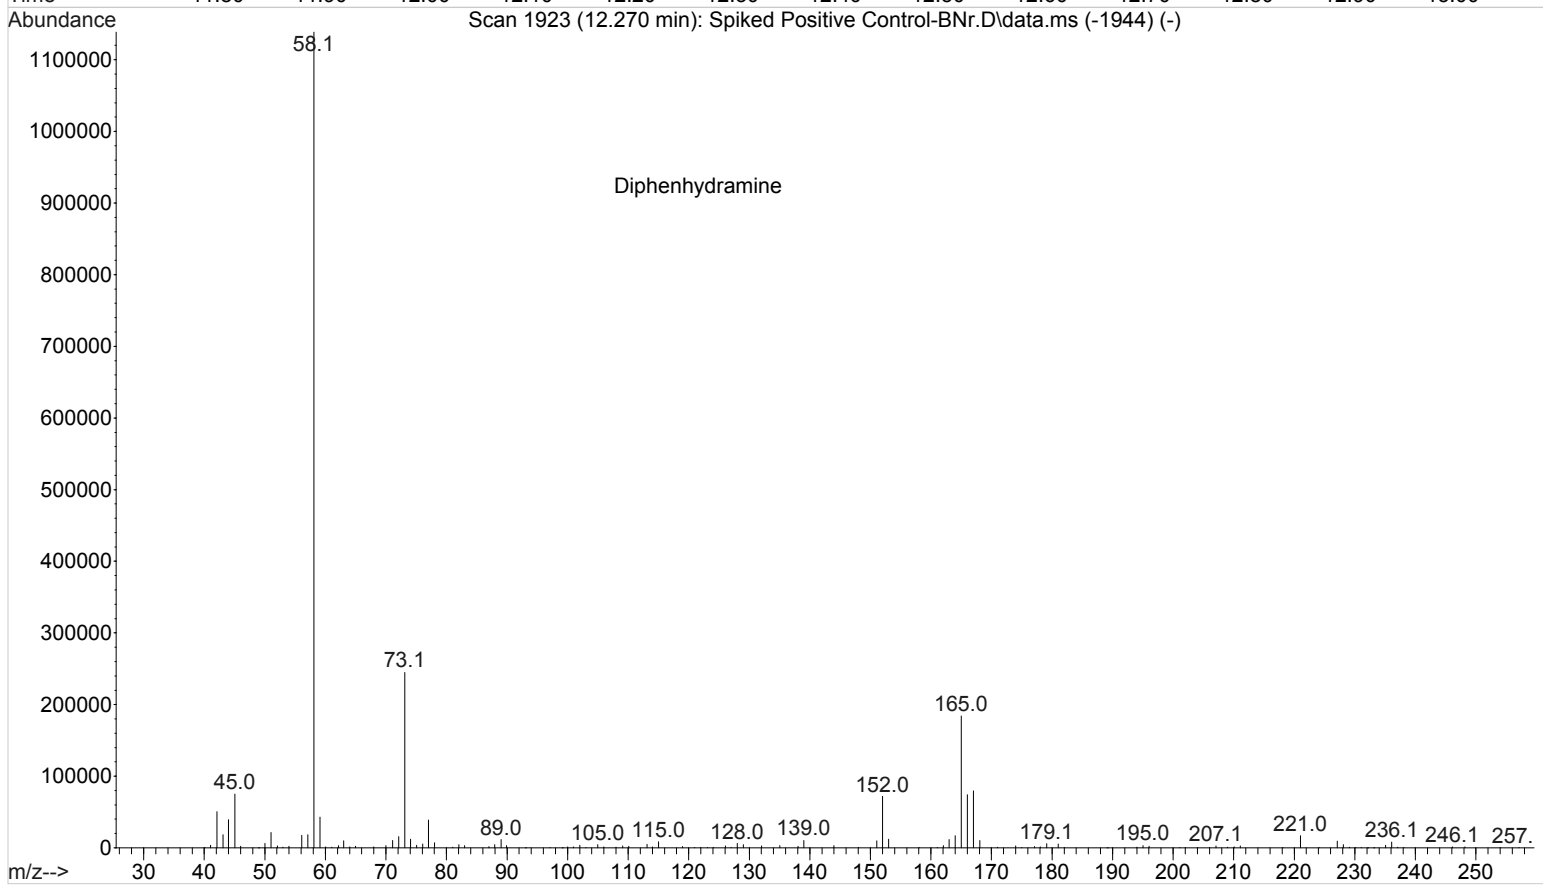
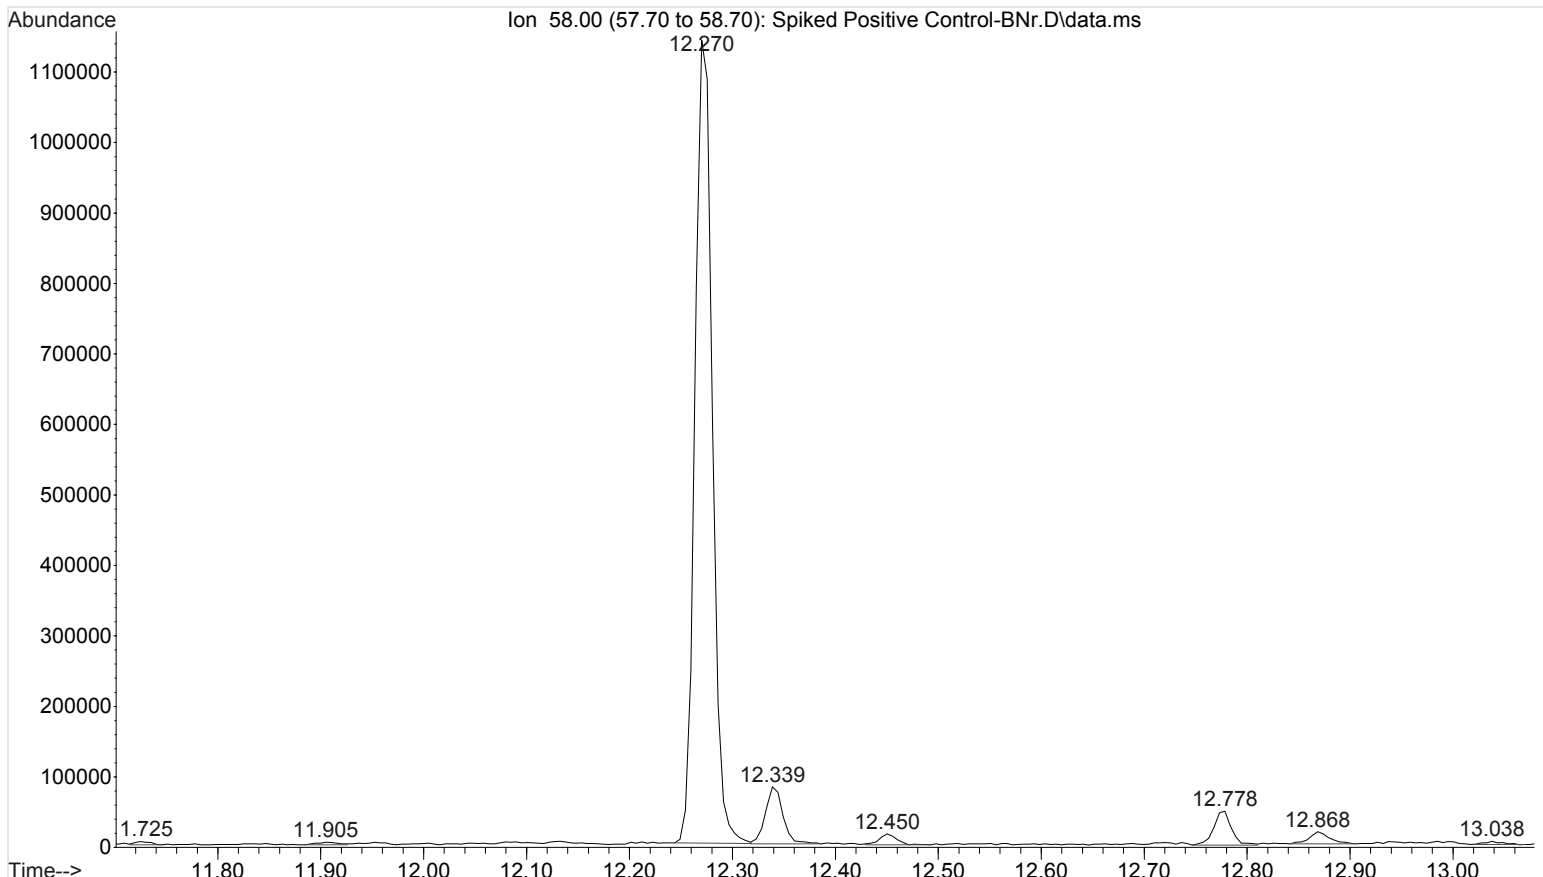


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Spiked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 18:33 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

9

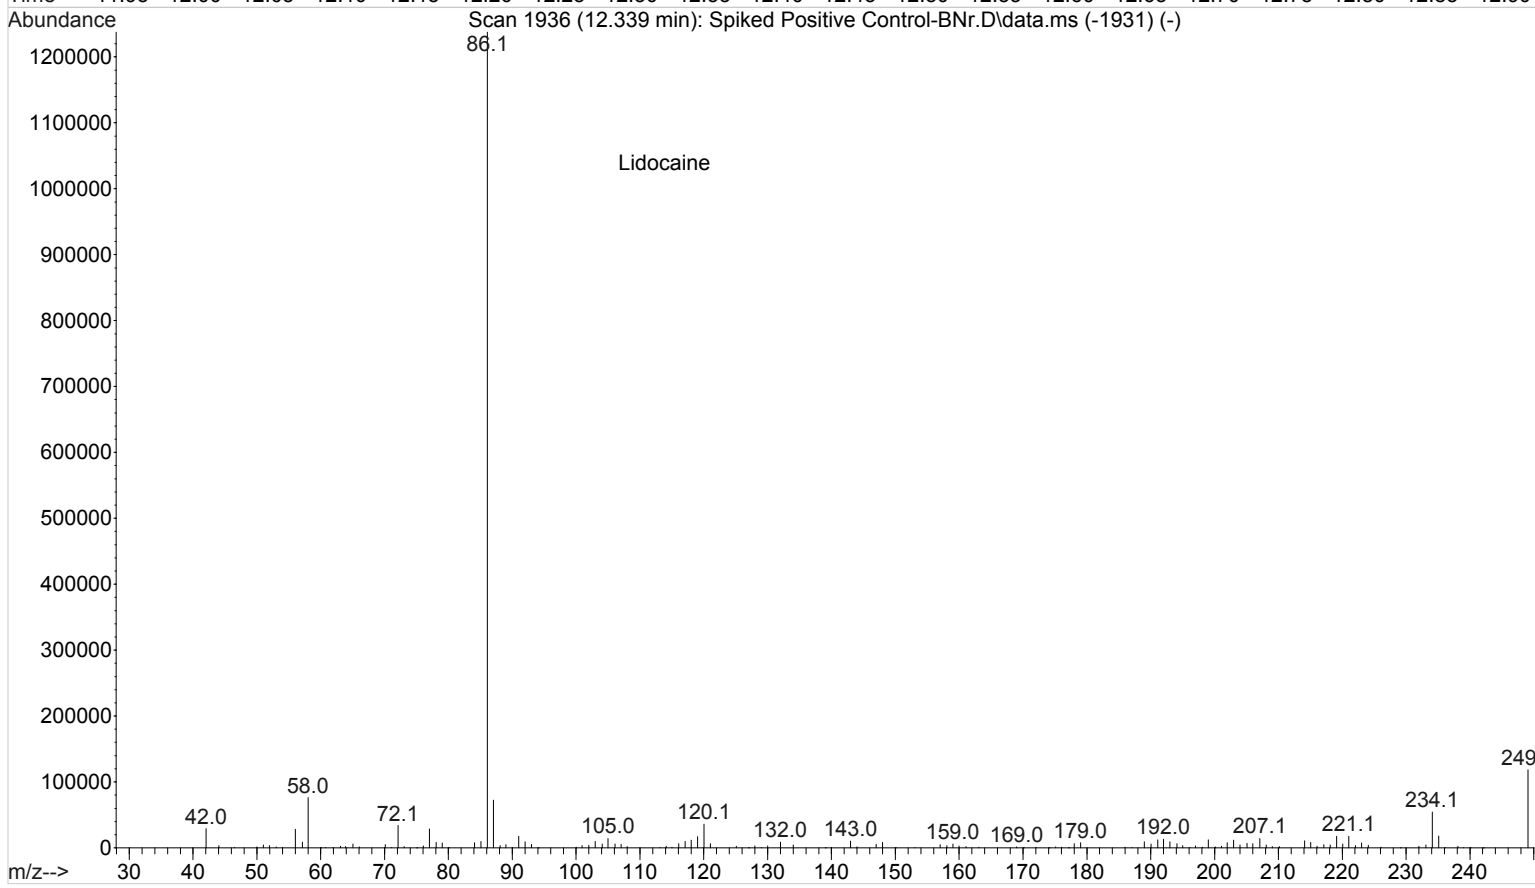
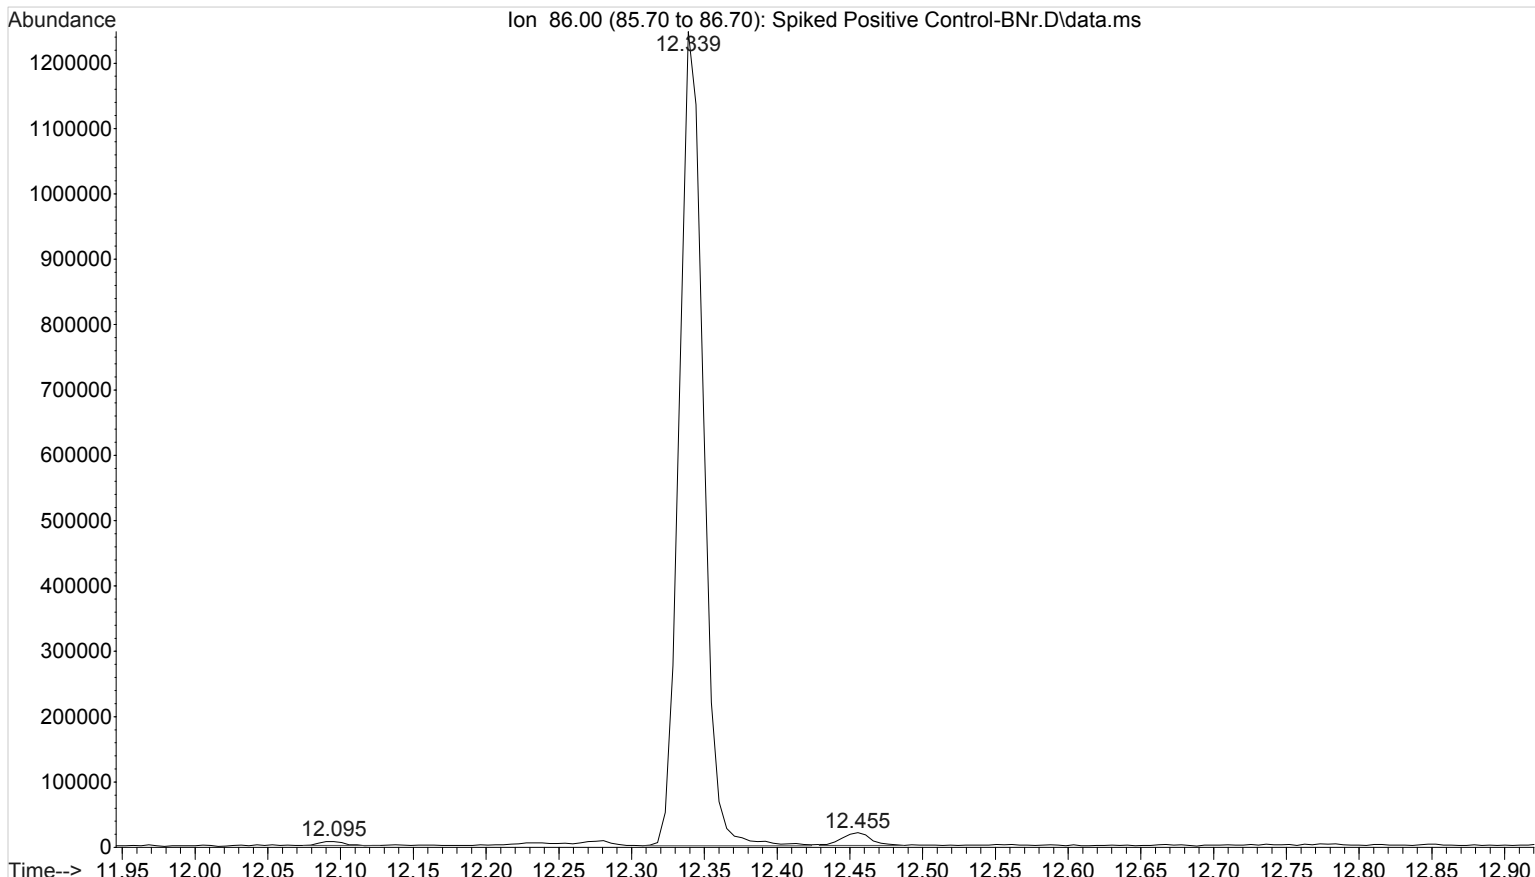


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Spiked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 18:33 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

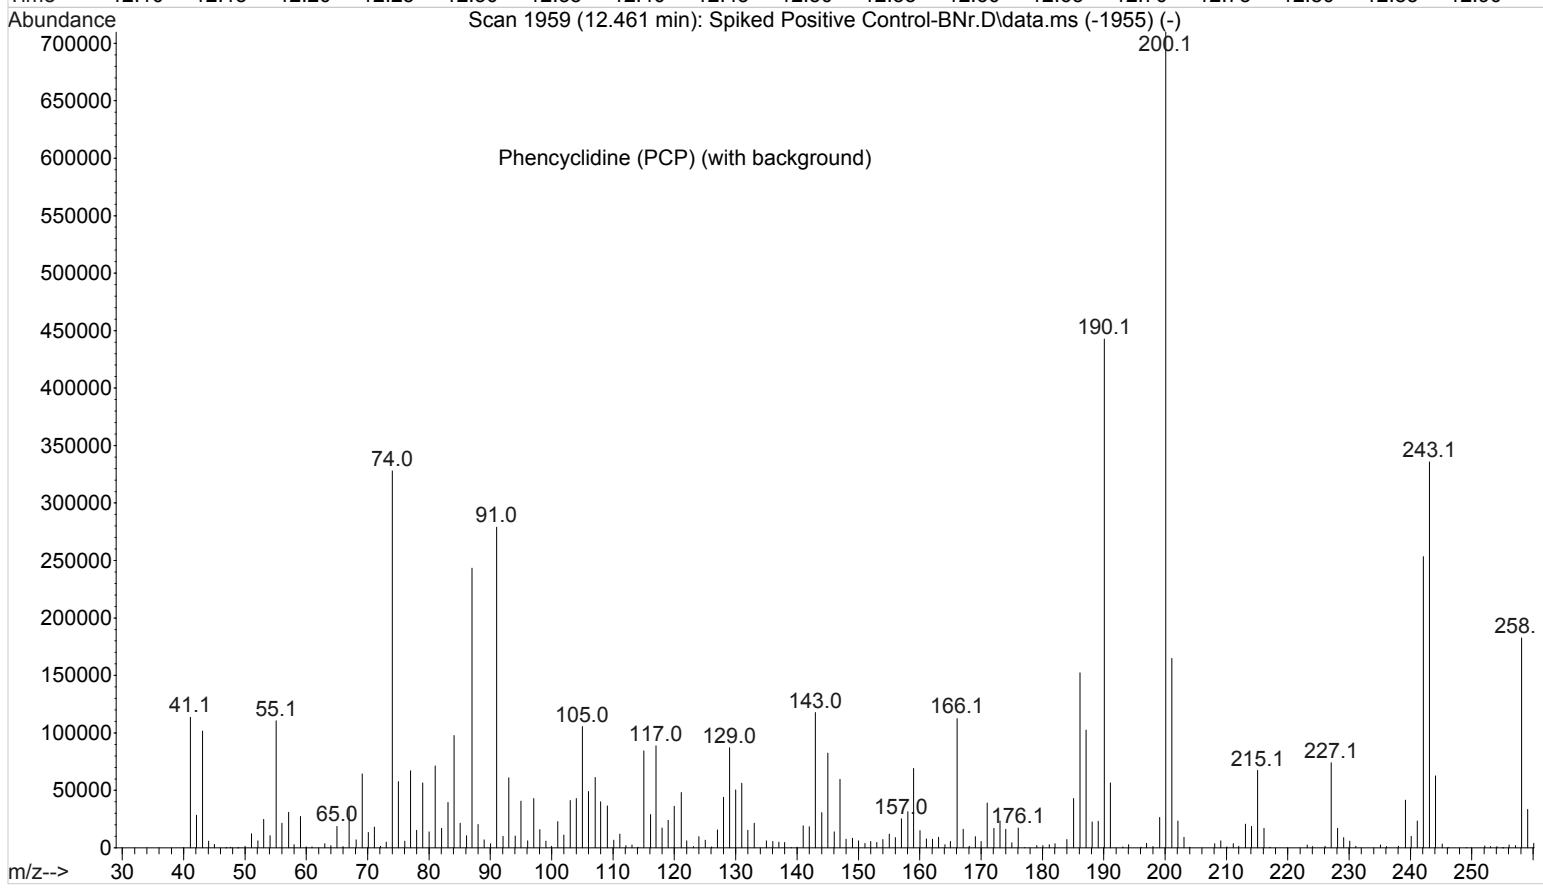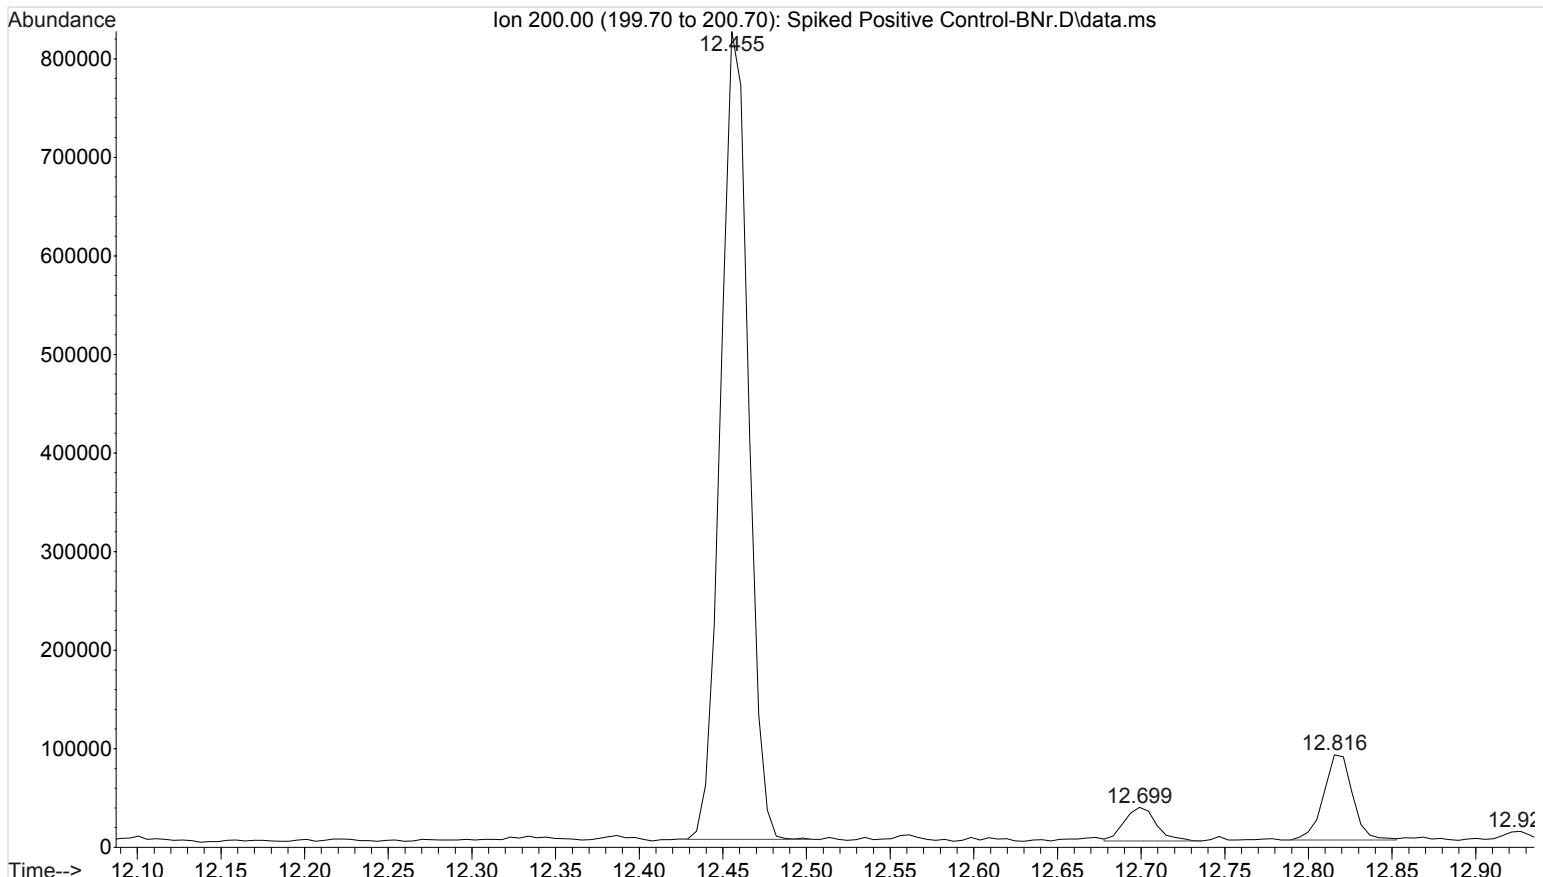



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Spiked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 18:33 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

9

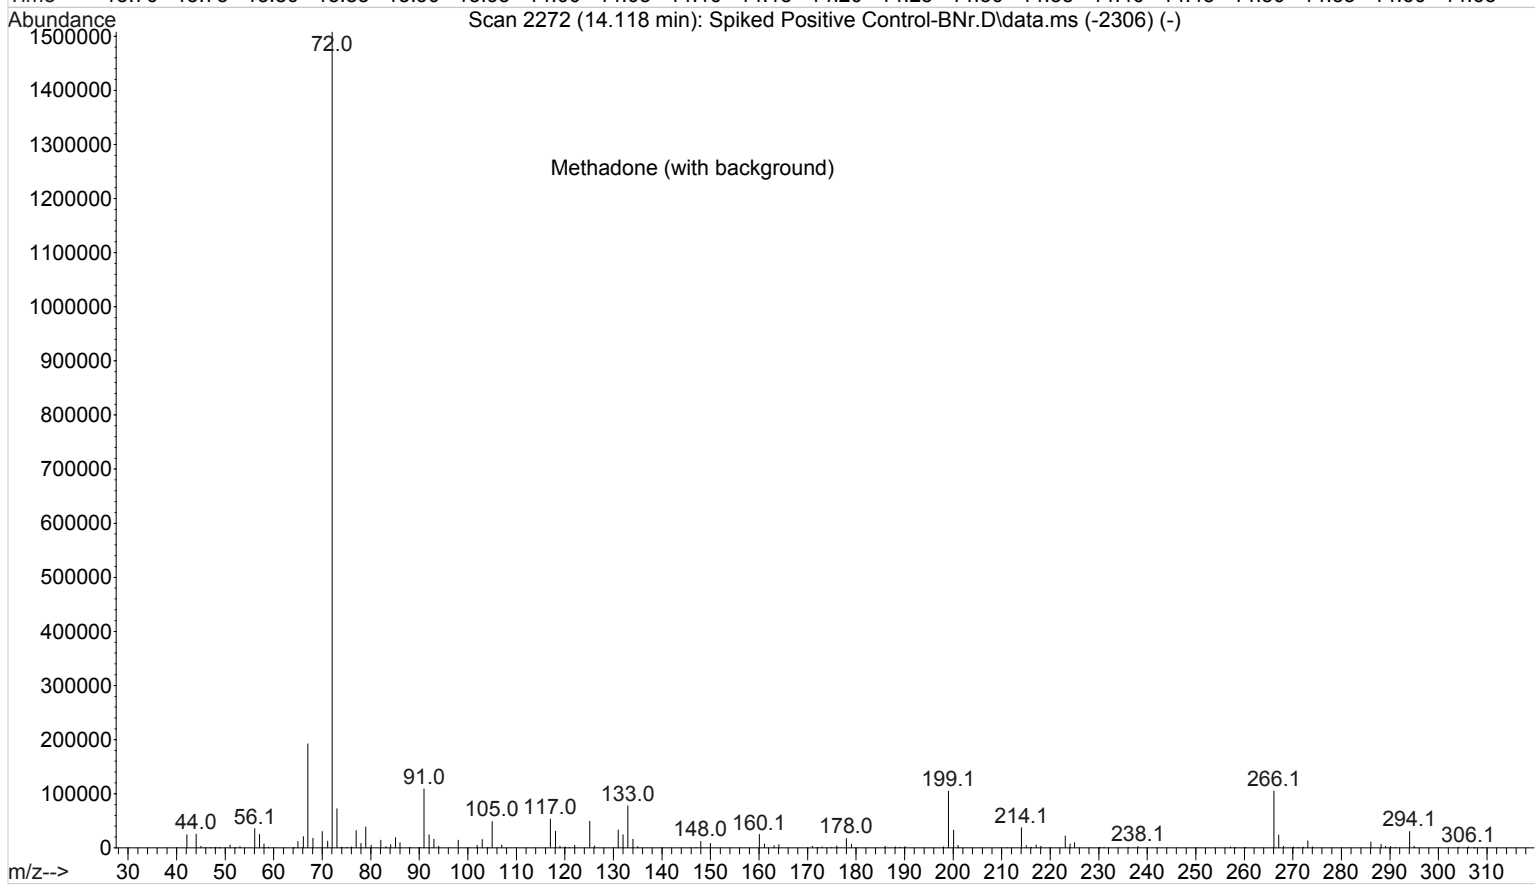
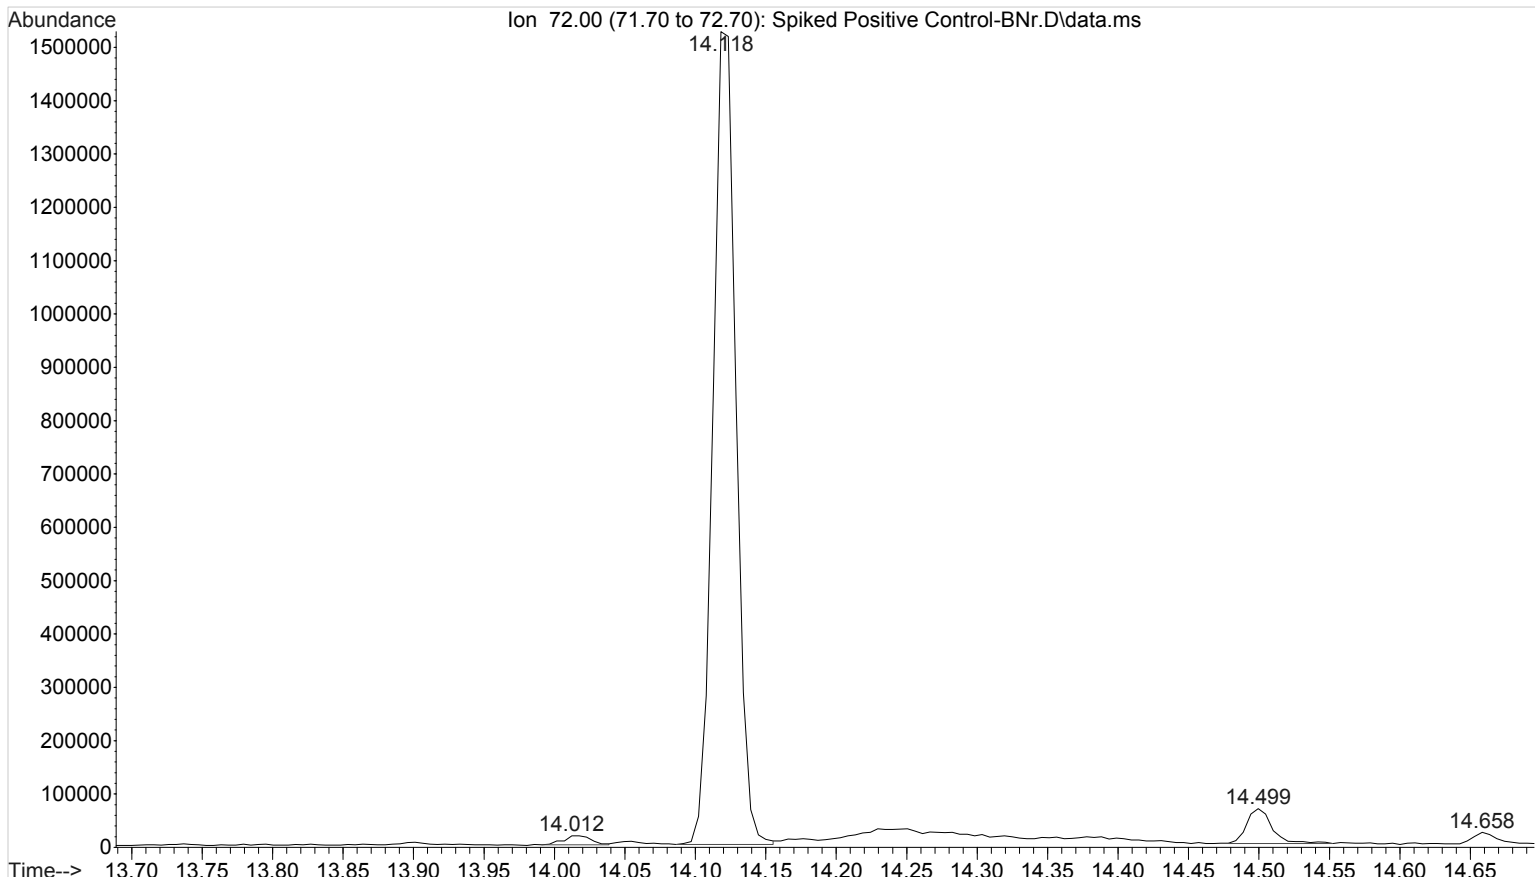


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Spiked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 18:33 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

9

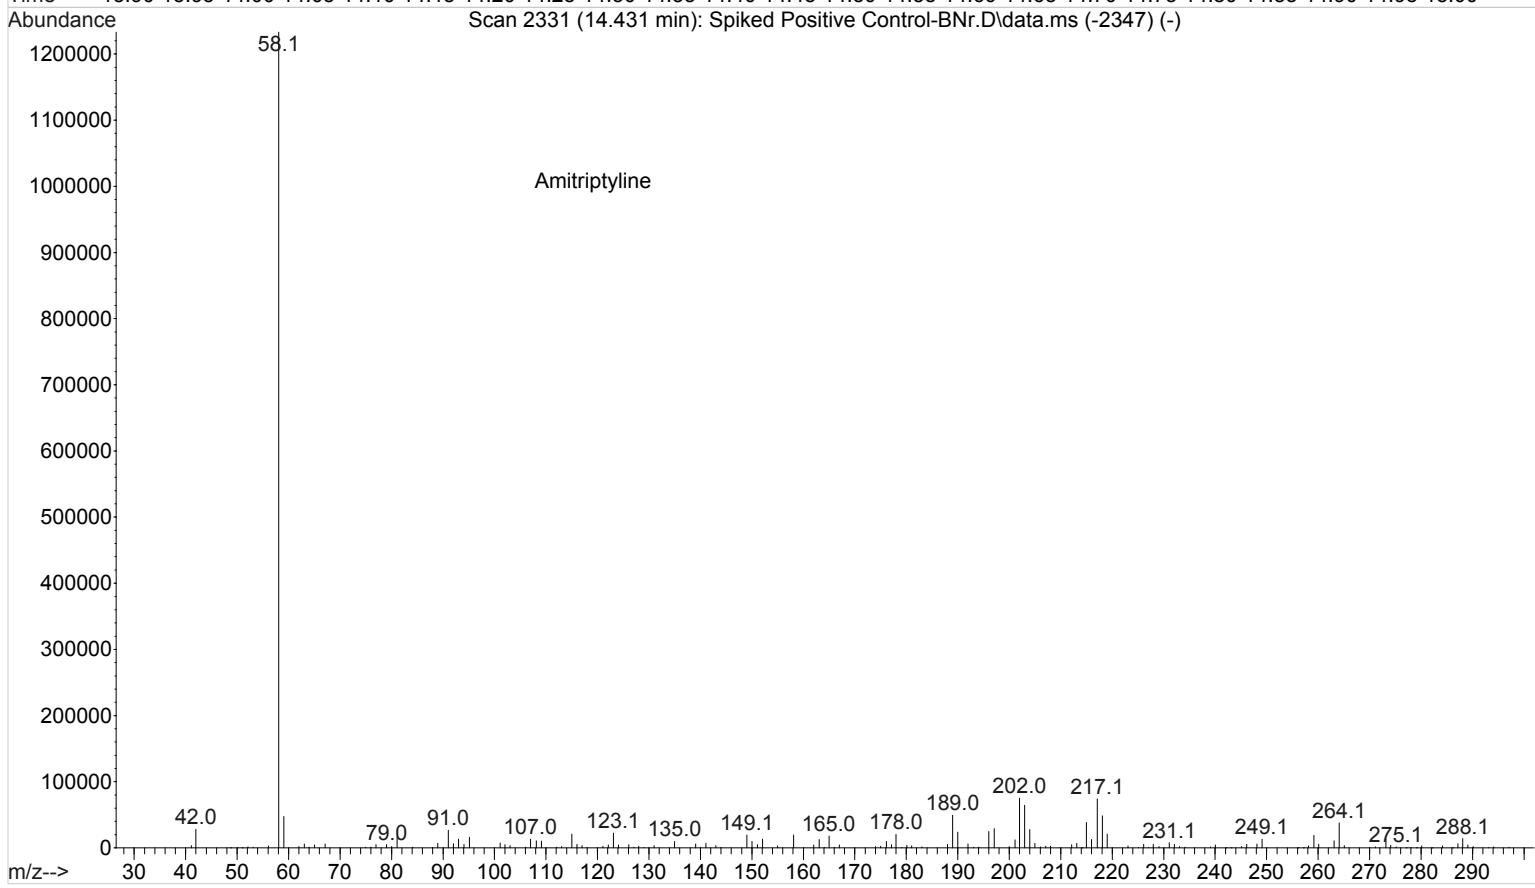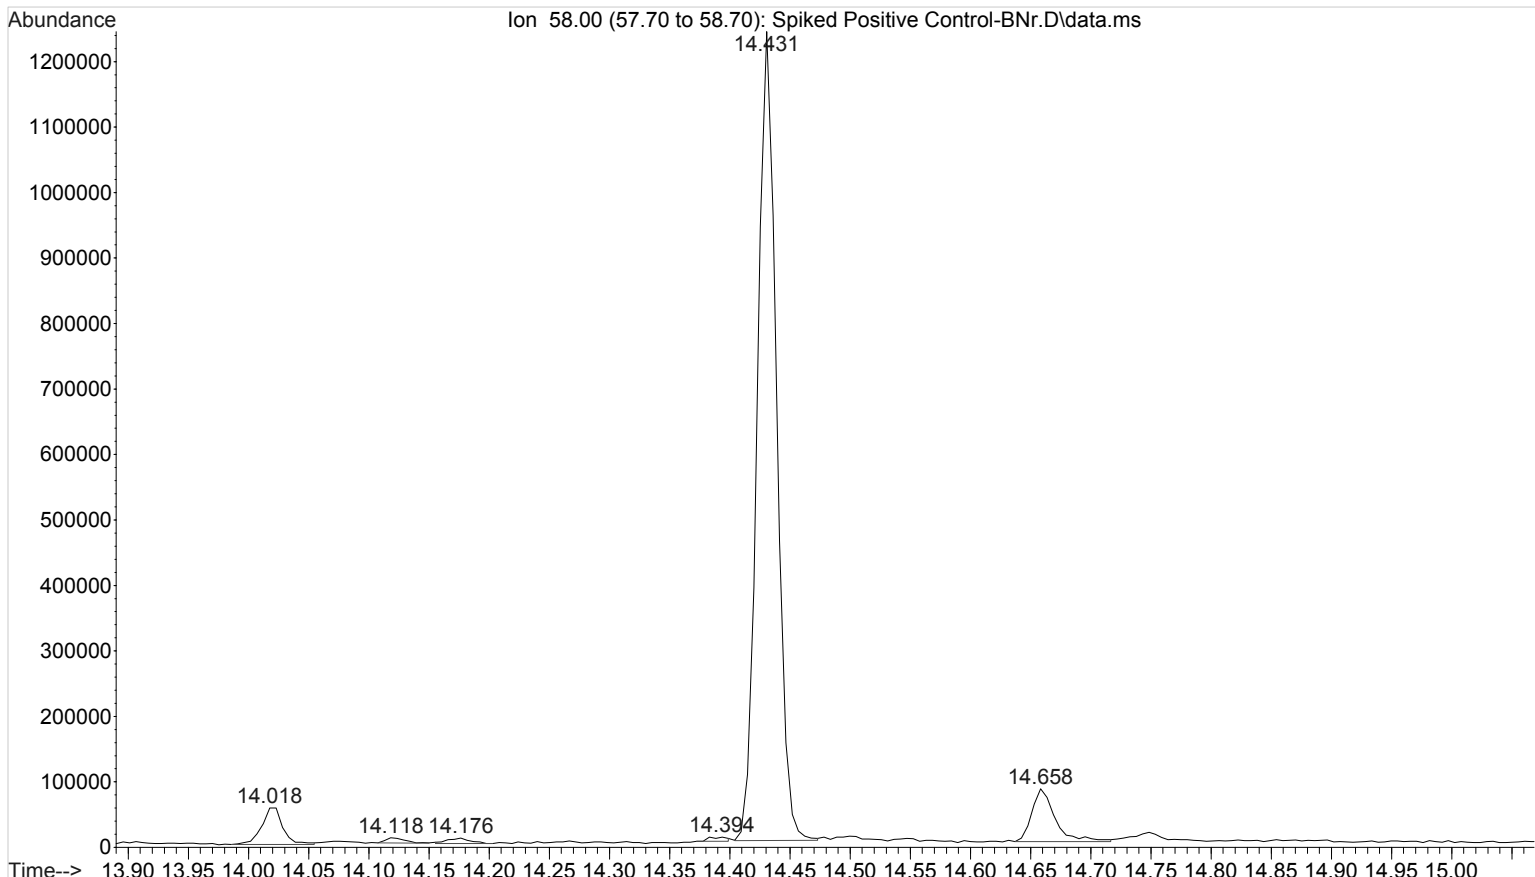

File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Spiked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 18:33 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

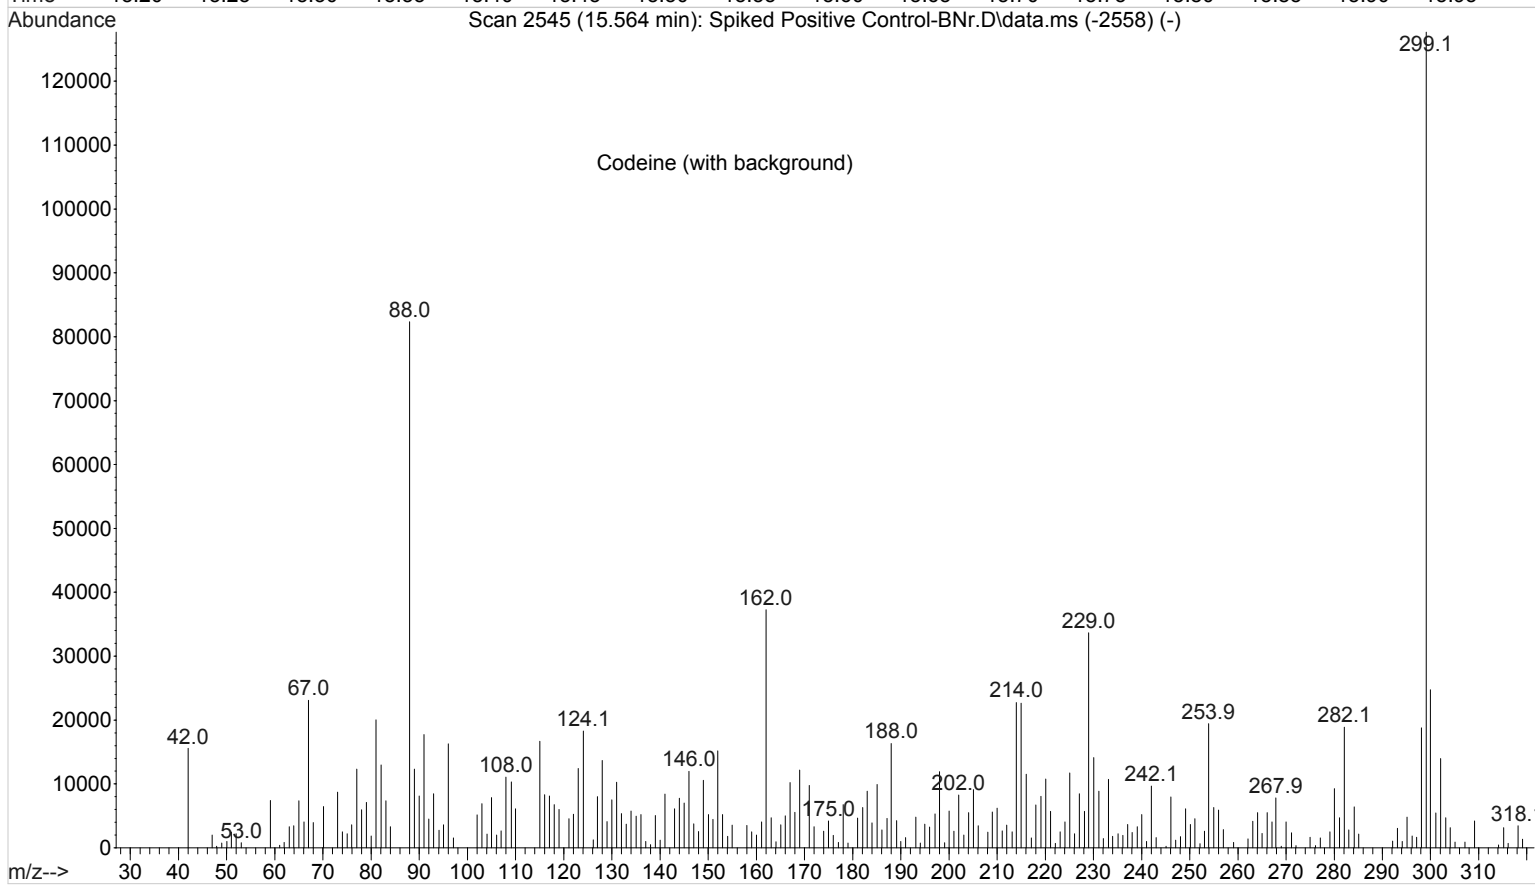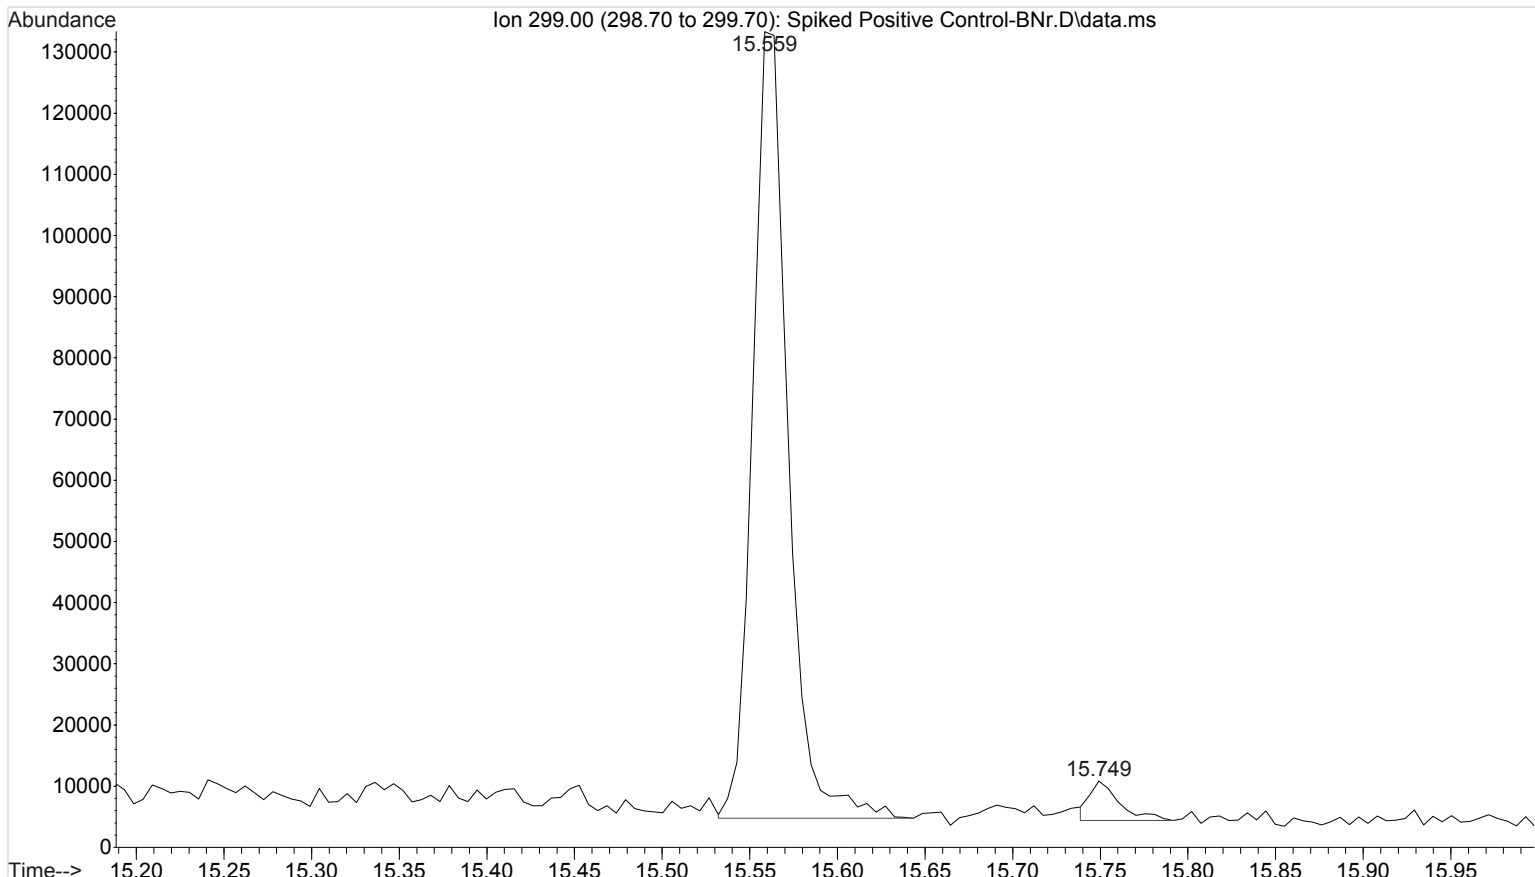

File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\071416
... \Spiked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 14 Jul 2016 18:33 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

