
























Worklist: 1236

<u>LAB_CASE</u>	<u>ITEM</u>	<u>TASK_ID</u>	<u>DESCRIPTION</u>	
M2016-0837	1	53264	3.6.1 Blood base neutral confirr	
M2016-0911	1	52215	3.6.1 Blood base neutral confirr	
M2016-1177	5	53789	3.6.1 Blood base neutral confirr	
M2016-1250	1	53660	3.6.1 Blood base neutral confirr	
M2016-1288	1	53900	3.6.1 Blood base neutral confirr	
P2016-0548	1	52174	3.6.1 Blood base neutral confirr	
P2016-0550	1	52197	3.6.1 Blood base neutral confirr	
P2016-0571	1	52377	3.6.1 Blood base neutral confirr	
P2016-0573	1	52388	3.6.1 Blood base neutral confirr	
P2016-0587	1	52448	3.6.1 Blood base neutral confirr	
P2016-0641	1	52610	3.6.1 Blood base neutral confirr	
P2016-0642	1	52618	3.6.1 Blood base neutral confirr	
P2016-0656	1	52734	3.6.1 Blood base neutral confirr	
P2016-0668	1	52840	3.6.1 Blood base neutral confirr	
P2016-0679	1	52935	3.6.1 Blood base neutral confirr	
P2016-0683	1	52968	3.6.1 Blood base neutral confirr	
P2016-0693	1	53037	3.6.1 Blood base neutral confirr	
P2016-0694	1	53043	3.6.1 Blood base neutral confirr	
P2016-0752	1	53407	3.6.1 Blood base neutral confirr	
P2016-0753	1	53410	3.6.1 Blood base neutral confirr	
P2016-0761	1	53511	3.6.1 Blood base neutral confirr	
P2016-0791	1	53786	3.6.1 Blood base neutral confirr	
P2016-0865	1	54475	3.6.1 Blood base neutral confirr	

**Worklist: 1236**

<u>LAB CASE</u>	<u>ITEM</u>	<u>TASK ID</u>	<u>DESCRIPTION</u>
P2016-0880	1	54506	3.6.1 Blood base neutral confirr
P2016-1006	1	55267	3.6.1 Blood base neutral confirr



reviewed 8/22/16

A handwritten signature in green ink, consisting of several overlapping loops and a long horizontal stroke extending to the right.

simulate\_sequence.log  
 Simulate Run Sequence Tue Aug 09 07:53:52 2016

Instrument Name: Major Mass Spec  
 Sequence File: C:\Users\ISPuser\Desktop\Sequences\CS-BNSB080516.sequence.xml  
 Comment: MassHunter sequence  
 Operator: ISP\datastor  
 Data Path: D:\DATA\CDS\2016\080516\  
 Method Path: C:\Users\datastor\Desktop\OP Methods\

Line	Type	Vials	DataFile	Sample Name
Acquisition Method: BNSB120510.M				
1)	Sample	100	Prerun Solvent Blank	Pre-run Solvent Blank
2)	Sample	1	Negative Control-BN	Negative Control -
...	1013			
3)	Sample	2	Spiked Positive Control-BN	Positive Control
4)	Sample	99	prBLK2	Solvent Blank
Acquisition Method: GBT092509-Delta EMV.M				
5)	Sample	100	Prerun Solvent Blankr	Pre-run Solvent Blank
6)	Sample	1	Negative Control-BNr	Negative Control -
...	1013			
7)	Sample	2	Spiked Positive Control-BNr	Positive Control
8)	Sample	99	prBLK2r	Solvent Blank
Acquisition Method: BNSB120510.M				
9)	Sample	100	M2016-0837-1-BNBLK	Lab No.: M2016-0837-1
10)	Sample	3	M2016-0837-1-BN	Lab No.: M2016-0837-1
Acquisition Method: GBT092509-Delta EMV.M				
11)	Sample	3	M2016-0837-1-BNr	Lab No.: M2016-0837-1
Acquisition Method: BNSB120510.M				
12)	Sample	100	M2016-0911-1-BNBLK	Lab No.: M2016-0911-1
13)	Sample	4	M2016-0911-1-BN	Lab No.: M2016-0911-1
Acquisition Method: GBT092509-Delta EMV.M				
14)	Sample	4	M2016-0911-1-BNr	Lab No.: M2016-0911-1
Acquisition Method: BNSB120510.M				
15)	Sample	100	M2016-1177-5-BNBLK	Lab No.: M2016-1177-5
16)	Sample	5	M2016-1177-5-BN	Lab No.: M2016-1177-5
Acquisition Method: GBT092509-Delta EMV.M				
17)	Sample	5	M2016-1177-5-BNr	Lab No.: M2016-1177-5
Acquisition Method: BNSB120510.M				
18)	Sample	100	M2016-1250-1-BNBLK	Lab No.: M2016-1250-1
19)	Sample	6	M2016-1250-1-BN	Lab No.: M2016-1250-1
Acquisition Method: GBT092509-Delta EMV.M				
20)	Sample	6	M2016-1250-1-BNr	Lab No.: M2016-1250-1
Acquisition Method: BNSB120510.M				
21)	Sample	100	M2016-1288-1-BNBLK	Lab No.: M2016-1288-1
22)	Sample	7	M2016-1288-1-BN	Lab No.: M2016-1288-1
Acquisition Method: GBT092509-Delta EMV.M				
23)	Sample	7	M2016-1288-1-BNr	Lab No.: M2016-1288-1
Acquisition Method: BNSB120510.M				
24)	Sample	100	P2016-0548-1-BNBLK	Lab No.: P2016-0548-1
25)	Sample	8	P2016-0548-1-BN	Lab No.: P2016-0548-1
Acquisition Method: GBT092509-Delta EMV.M				
26)	Sample	8	P2016-0548-1-BNr	Lab No.: P2016-0548-1

## simulate\_sequence.log

Acquisition Method:	BNSB120510.M		
27) Sample	100	P2016-0550-1-BNBLK	Lab No.: P2016-0550-1
28) Sample	9	P2016-0550-1-BN	Lab No.: P2016-0550-1
Acquisition Method:	GBT092509-Delta EMV.M		
29) Sample	9	P2016-0550-1-BNr	Lab No.: P2016-0550-1
Acquisition Method:	BNSB120510.M		
30) Sample	100	P2016-0571-1-BNBLK	Lab No.: P2016-0571-1
31) Sample	10	P2016-0571-1-BN	Lab No.: P2016-0571-1
Acquisition Method:	GBT092509-Delta EMV.M		
32) Sample	10	P2016-0571-1-BNr	Lab No.: P2016-0571-1
Acquisition Method:	BNSB120510.M		
33) Sample	100	P2016-0573-1-BNBLK	Lab No.: P2016-0573-1
34) Sample	11	P2016-0573-1-BN	Lab No.: P2016-0573-1
Acquisition Method:	GBT092509-Delta EMV.M		
35) Sample	11	P2016-0573-1-BNr	Lab No.: P2016-0573-1
Acquisition Method:	BNSB120510.M		
36) Sample	100	P2016-0587-1-BNBLK	Lab No.: P2016-0587-1
37) Sample	12	P2016-0587-1-BN	Lab No.: P2016-0587-1
Acquisition Method:	GBT092509-Delta EMV.M		
38) Sample	12	P2016-0587-1-BNr	Lab No.: P2016-0587-1
Acquisition Method:	BNSB120510.M		
39) Sample	100	P2016-0641-1-BNBLK	Lab No.: P2016-0641-1
40) Sample	13	P2016-0641-1-BN	Lab No.: P2016-0641-1
Acquisition Method:	GBT092509-Delta EMV.M		
41) Sample	13	P2016-0641-1-BNr	Lab No.: P2016-0641-1
Acquisition Method:	BNSB120510.M		
42) Sample	100	P2016-0642-1-BNBLK	Lab No.: P2016-0642-1
43) Sample	14	P2016-0642-1-BN	Lab No.: P2016-0642-1
Acquisition Method:	GBT092509-Delta EMV.M		
44) Sample	14	P2016-0642-1-BNr	Lab No.: P2016-0642-1
Acquisition Method:	BNSB120510.M		
45) Sample	100	P2016-0656-1-BNBLK	Lab No.: P2016-0656-1
46) Sample	15	P2016-0656-1-BN	Lab No.: P2016-0656-1
Acquisition Method:	GBT092509-Delta EMV.M		
47) Sample	15	P2016-0656-1-BNr	Lab No.: P2016-0656-1
Acquisition Method:	BNSB120510.M		
48) Sample	99	P2016-0668-1-BNBLK	Lab No.: P2016-0668-1
49) Sample	16	P2016-0668-1-BN	Lab No.: P2016-0668-1
Acquisition Method:	GBT092509-Delta EMV.M		
50) Sample	16	P2016-0668-1-BNr	Lab No.: P2016-0668-1
Acquisition Method:	BNSB120510.M		
51) Sample	99	P2016-0679-1-BNBLK	Lab No.: P2016-0679-1
52) Sample	17	P2016-0679-1-BN	Lab No.: P2016-0679-1
Acquisition Method:	GBT092509-Delta EMV.M		
53) Sample	17	P2016-0679-1-BNr	Lab No.: P2016-0679-1
Acquisition Method:	BNSB120510.M		
54) Sample	99	P2016-0683-1-BNBLK	Lab No.: P2016-0683-1
55) Sample	18	P2016-0683-1-BN	Lab No.: P2016-0683-1

```

simulate_sequence.log
Acquisition Method: GBT092509-Delta EMV.M
56) Sample 18 P2016-0683-1-BNr Lab No.: P2016-0683-1

Acquisition Method: BNSB120510.M
57) Sample 99 P2016-0693-1-BNBLK Lab No.: P2016-0693-1
58) Sample 19 P2016-0693-1-BN Lab No.: P2016-0693-1

Acquisition Method: GBT092509-Delta EMV.M
59) Sample 19 P2016-0693-1-BNr Lab No.: P2016-0693-1

Acquisition Method: BNSB120510.M
60) Sample 99 P2016-0694-1-BNBLK Lab No.: P2016-0694-1
61) Sample 20 P2016-0694-1-BN Lab No.: P2016-0694-1

Acquisition Method: GBT092509-Delta EMV.M
62) Sample 20 P2016-0694-1-BNr Lab No.: P2016-0694-1

Acquisition Method: BNSB120510.M
63) Sample 99 P2016-0752-1-BNBLK Lab No.: P2016-0752-1
64) Sample 21 P2016-0752-1-BN Lab No.: P2016-0752-1

Acquisition Method: GBT092509-Delta EMV.M
65) Sample 21 P2016-0752-1-BNr Lab No.: P2016-0752-1

Acquisition Method: BNSB120510.M
66) Sample 99 P2016-0753-1-BNBLK Lab No.: P2016-0753-1
67) Sample 22 P2016-0753-1-BN Lab No.: P2016-0753-1

Acquisition Method: GBT092509-Delta EMV.M
68) Sample 22 P2016-0753-1-BNr Lab No.: P2016-0753-1

Acquisition Method: BNSB120510.M
69) Sample 99 P2016-0761-1-BNBLK Lab No.: P2016-0761-1
70) Sample 23 P2016-0761-1-BN Lab No.: P2016-0761-1

Acquisition Method: GBT092509-Delta EMV.M
71) Sample 23 P2016-0761-1-BNr Lab No.: P2016-0761-1

Acquisition Method: BNSB120510.M
72) Sample 99 P2016-0791-1-BNBLK Lab No.: P2016-0791-1
73) Sample 24 P2016-0791-1-BN Lab No.: P2016-0791-1

Acquisition Method: GBT092509-Delta EMV.M
74) Sample 24 P2016-0791-1-BNr Lab No.: P2016-0791-1

Acquisition Method: BNSB120510.M
75) Sample 99 P2016-0865-1-BNBLK Lab No.: P2016-0865-1
76) Sample 25 P2016-0865-1-BN Lab No.: P2016-0865-1

Acquisition Method: GBT092509-Delta EMV.M
77) Sample 25 P2016-0865-1-BNr Lab No.: P2016-0865-1

Acquisition Method: BNSB120510.M
78) Sample 99 P2016-0880-1-BNBLK Lab No.: P2016-0880-1
79) Sample 26 P2016-0880-1-BN Lab No.: P2016-0880-1

Acquisition Method: GBT092509-Delta EMV.M
80) Sample 26 P2016-0880-1-BNr Lab No.: P2016-0880-1

Acquisition Method: BNSB120510.M
81) Sample 99 P2016-1006-1-BNBLK Lab No.: P2016-1006-1
82) Sample 27 P2016-1006-1-BN Lab No.: P2016-1006-1

Acquisition Method: GBT092509-Delta EMV.M
83) Sample 27 P2016-1006-1-BNr Lab No.: P2016-1006-1

Acquisition Method: BNSB120510.M
84) Sample 99 POSTBLK BLK

```

simulate\_sequence.log

Acquisition Method: GBT092509-Delta EMV.M  
85) Sample 99 AFTER BLK  
megabytes Needed: 1893 Space on drive D: 227354  
Sequence Verification Done!

Analytical Method 3.6.1 & 3.6.7 QA Check List

---

Run Start Date: 08/05/2016

Analyst: CS

(Short GC/MS temperature program)

Positive Control Compound List


- Phentermine
- Methamphetamine
- Nicotine
- Meperidine
- Caffeine
- Diphenhydramine
- Lidocaine
- PCP
- Methadone
- Amitriptyline
- Codeine

Internal Standards

- Benzphetamine
- Papaverine

Optional back extraction **not** performed.  
Reconstituted in MeOH.


File :I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\080516  
 ... \Negative Control-BN.D  
 Operator : ISP\datastor  
 Instrument : Major Mass Spec  
 Acquired : 05 Aug 2016 15:56 using AcqMethod BNSB120510.M  
 Sample Name: Negative Control - Utak Lot B1013  
 Misc Info : Analytical Method 3.6.1

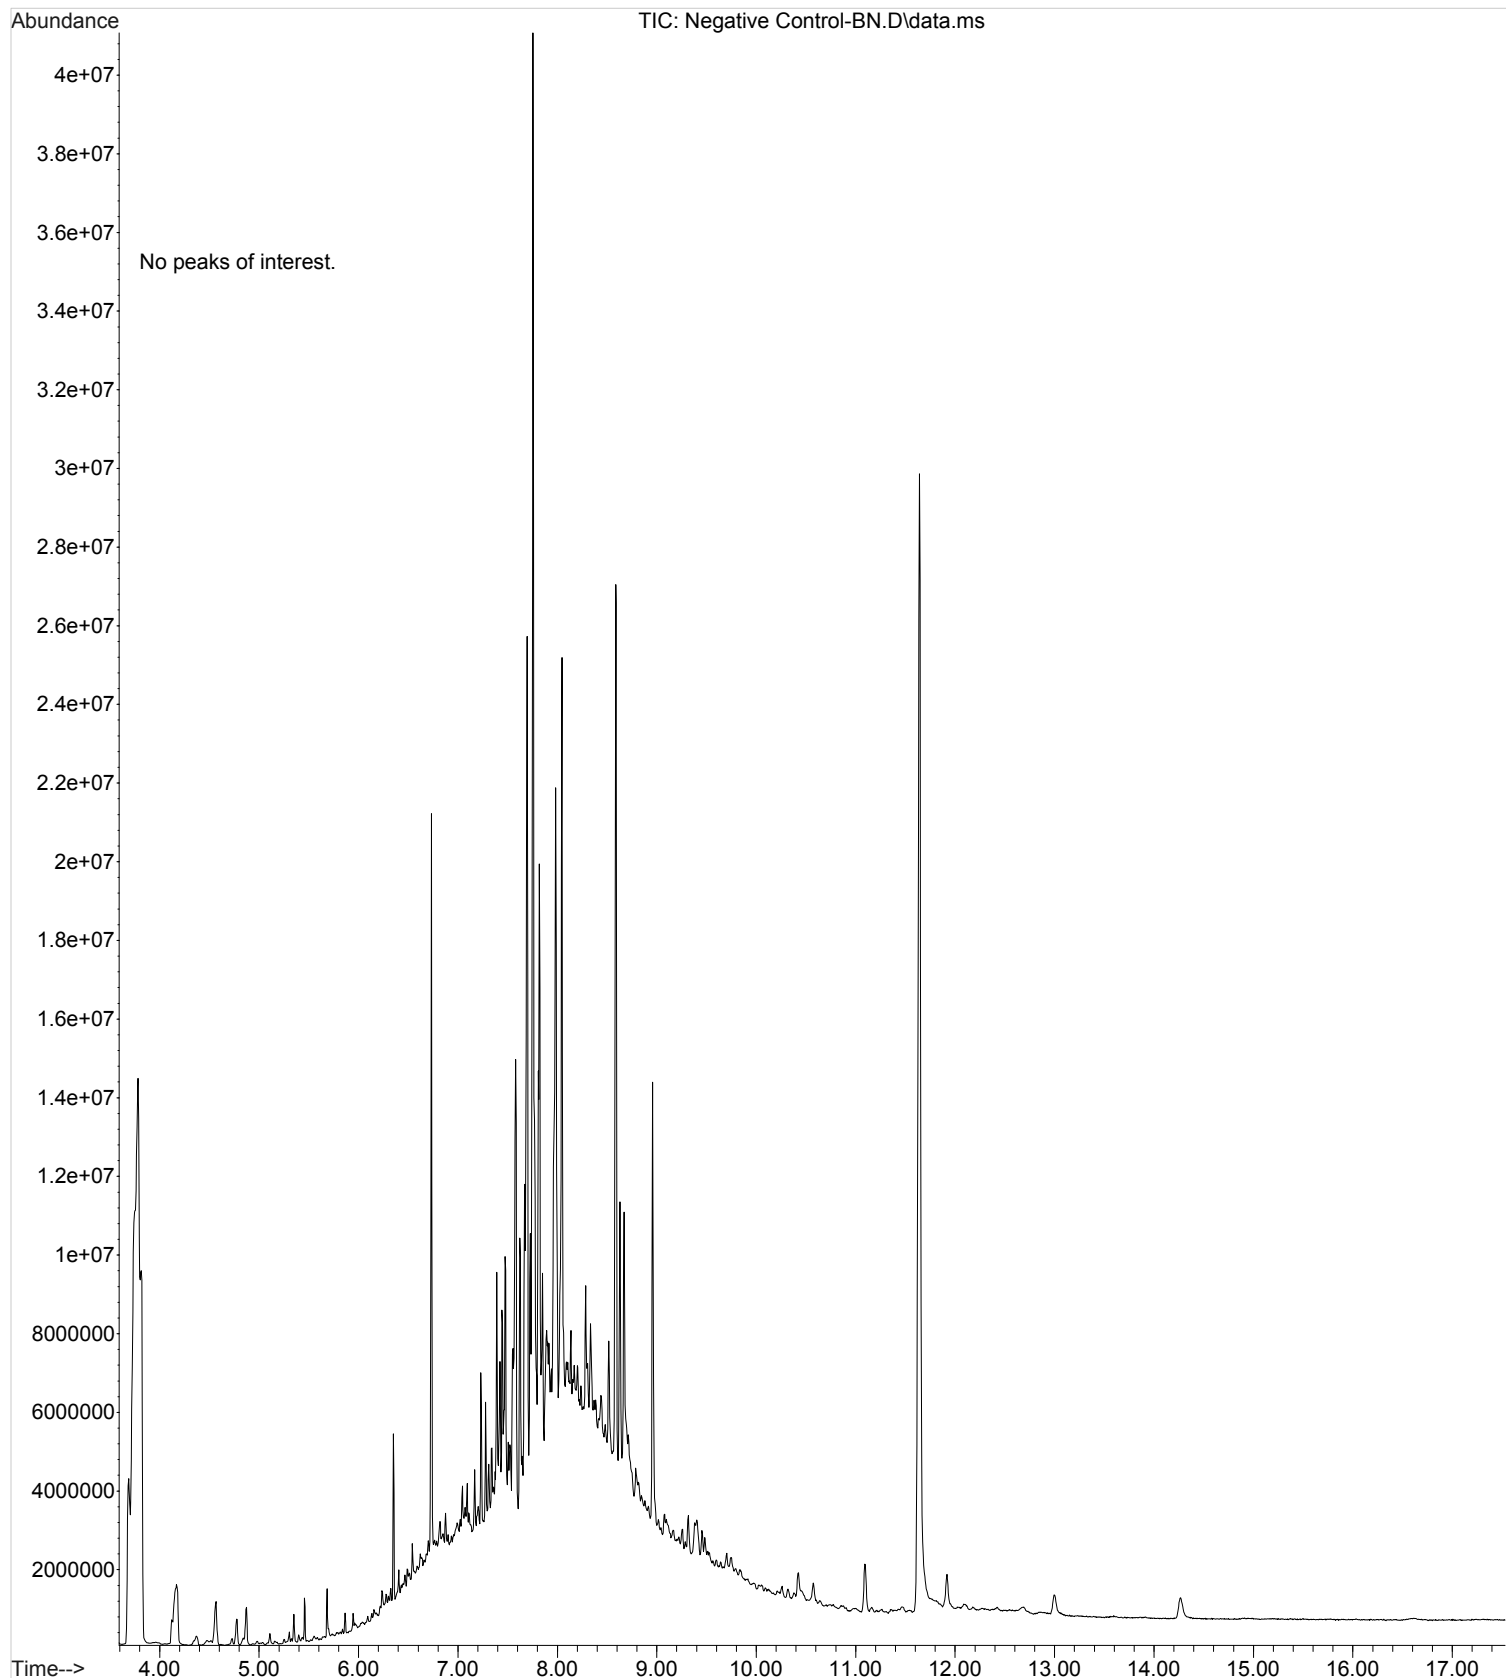





File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\080516  
... \Negative Control-BN.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 05 Aug 2016 15:56 using AcqMethod BNSB120510.M  
Sample Name: Negative Control - Utak Lot B1013  
Misc Info : Analytical Method 3.6.1

9


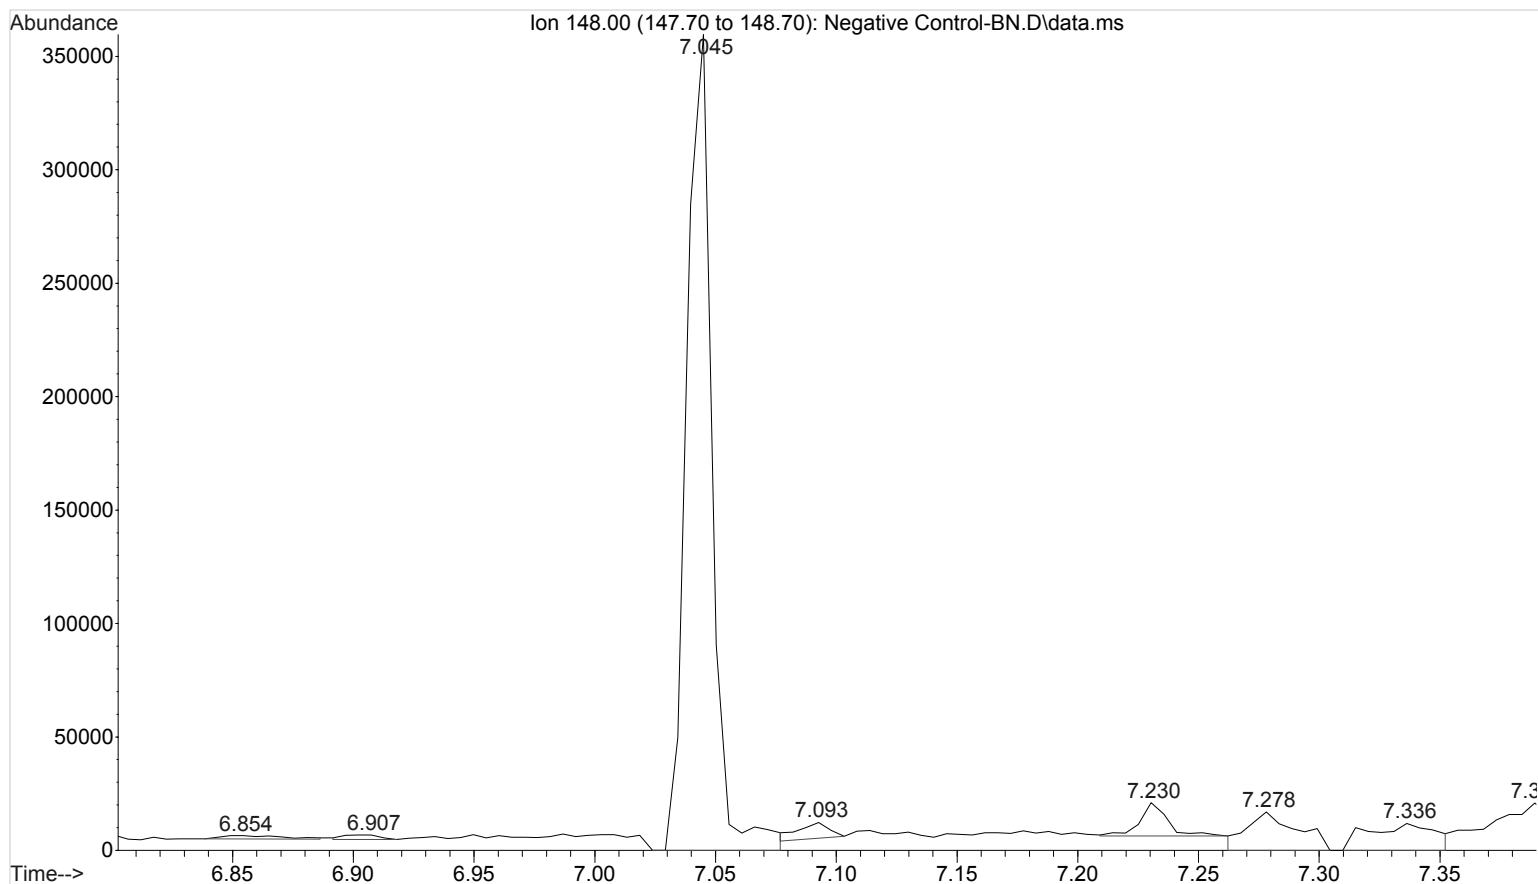


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\080516  
... \Negative Control-BN.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 05 Aug 2016 15:56 using AcqMethod BNSB120510.M  
Sample Name: Negative Control - Utak Lot B1013  
Misc Info : Analytical Method 3.6.1

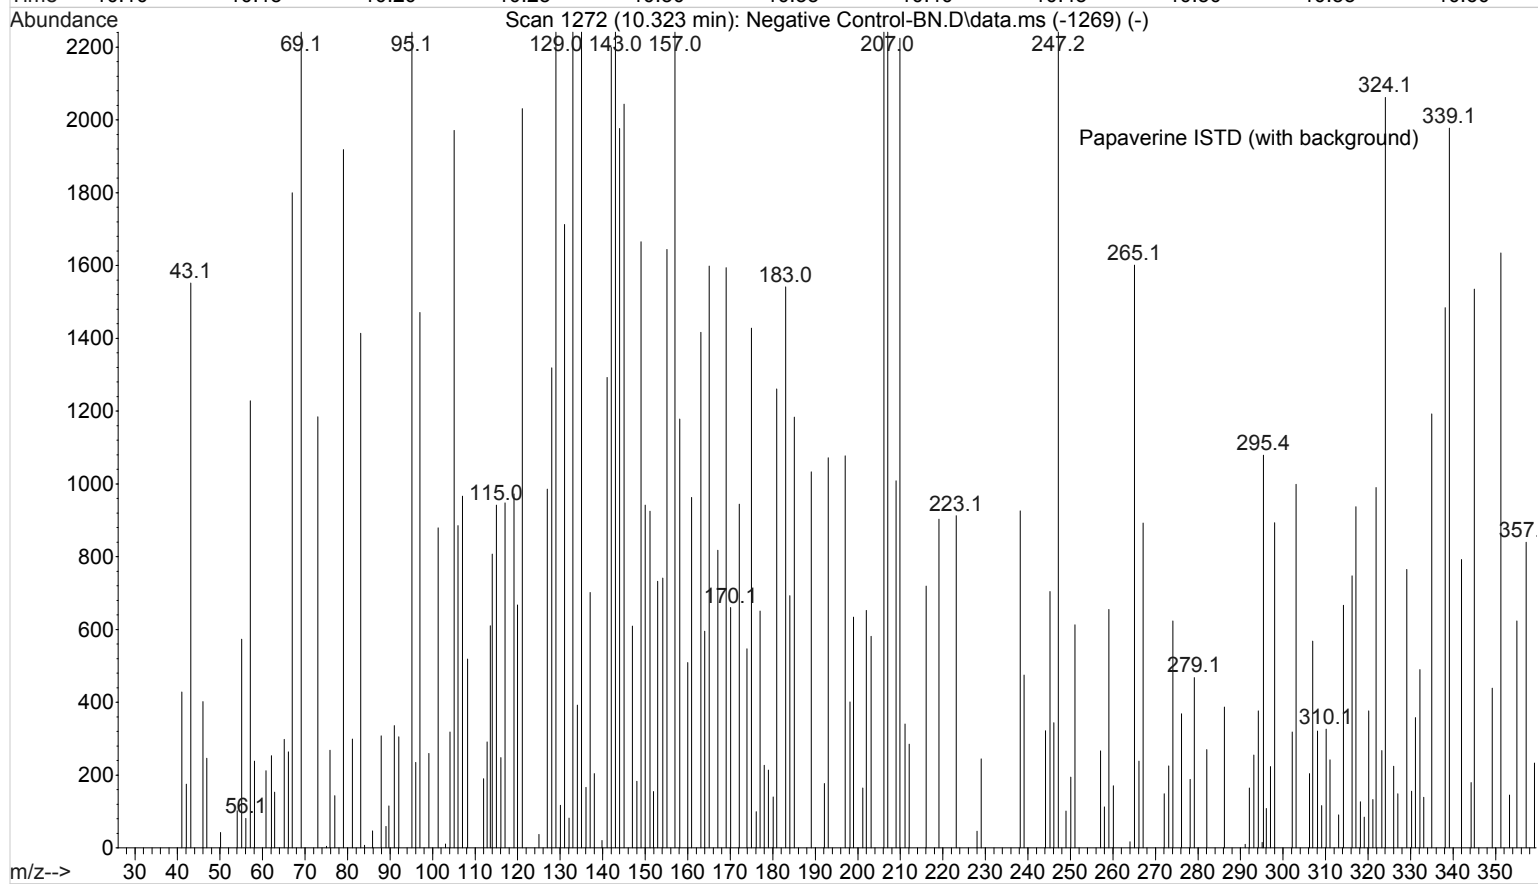
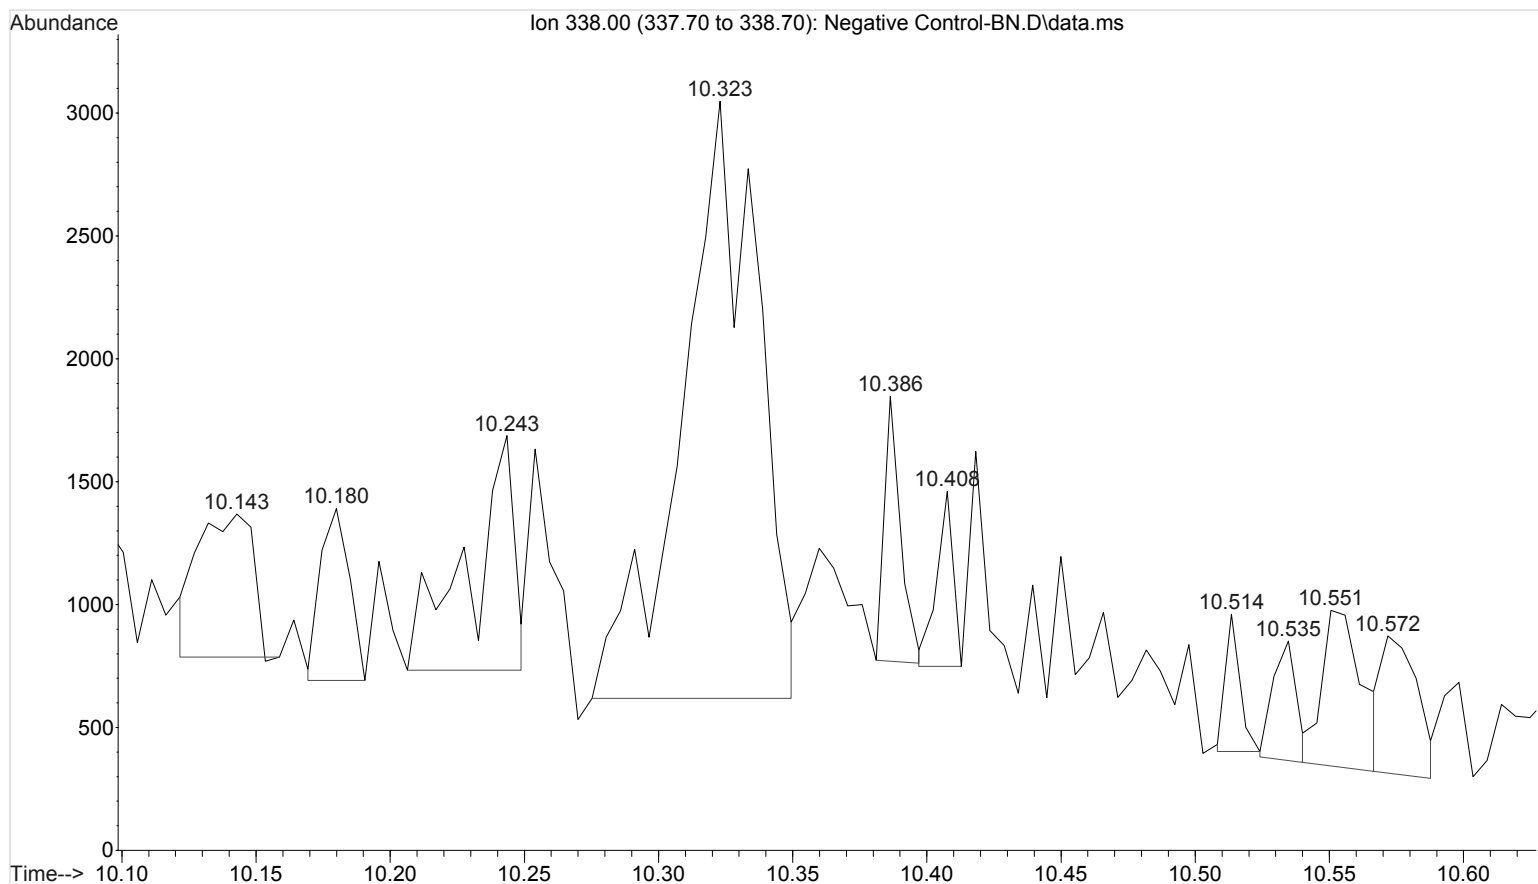


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\080516  
... \Spiked Positive Control-BN.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 05 Aug 2016 16:19 using AcqMethod BNSB120510.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215



59

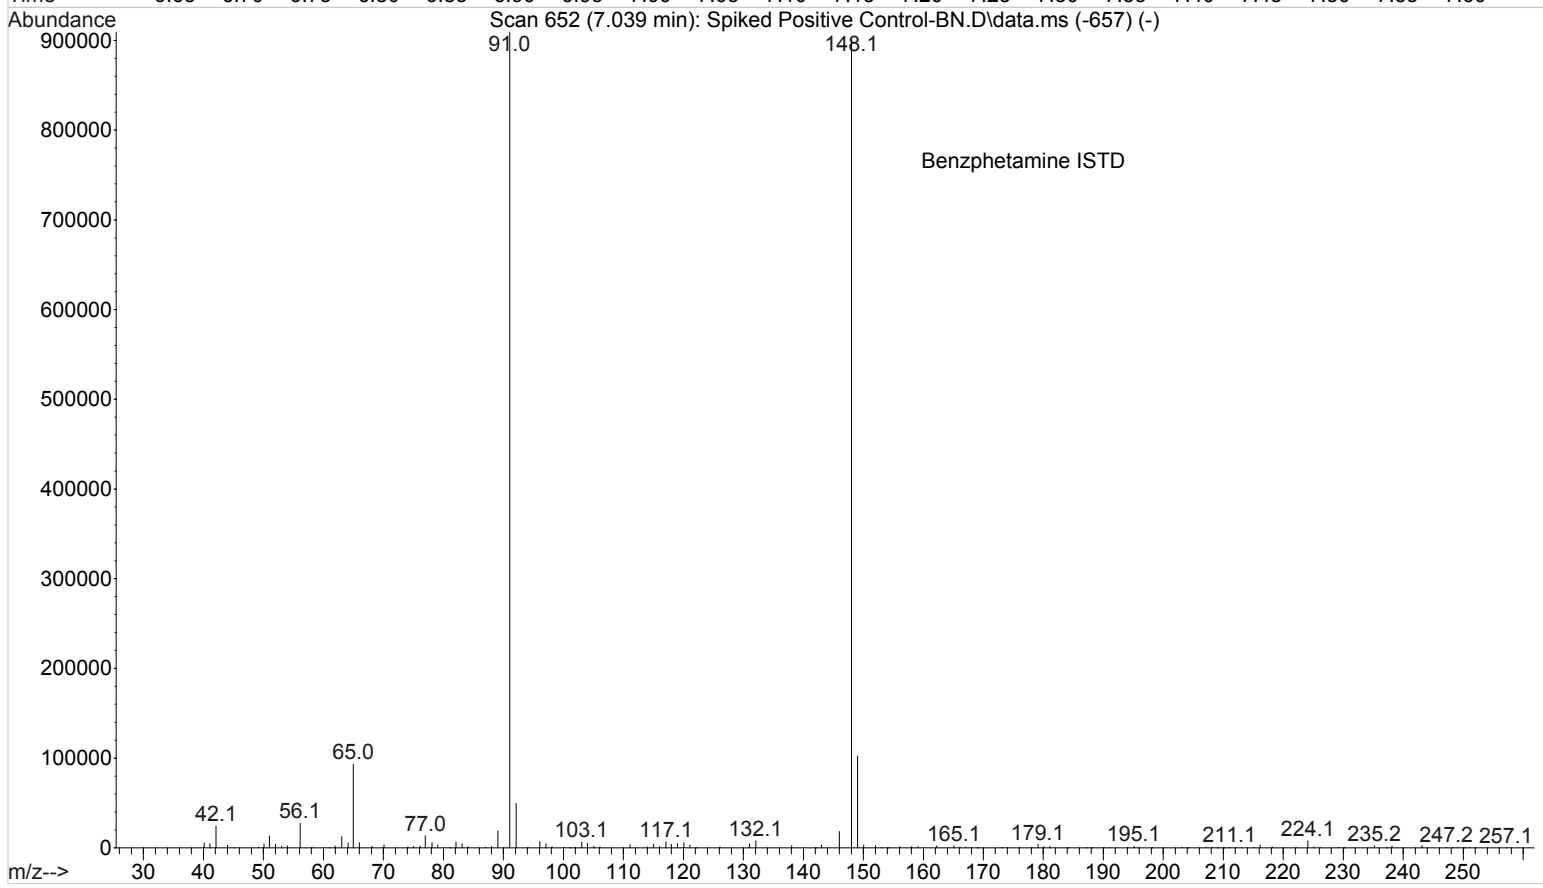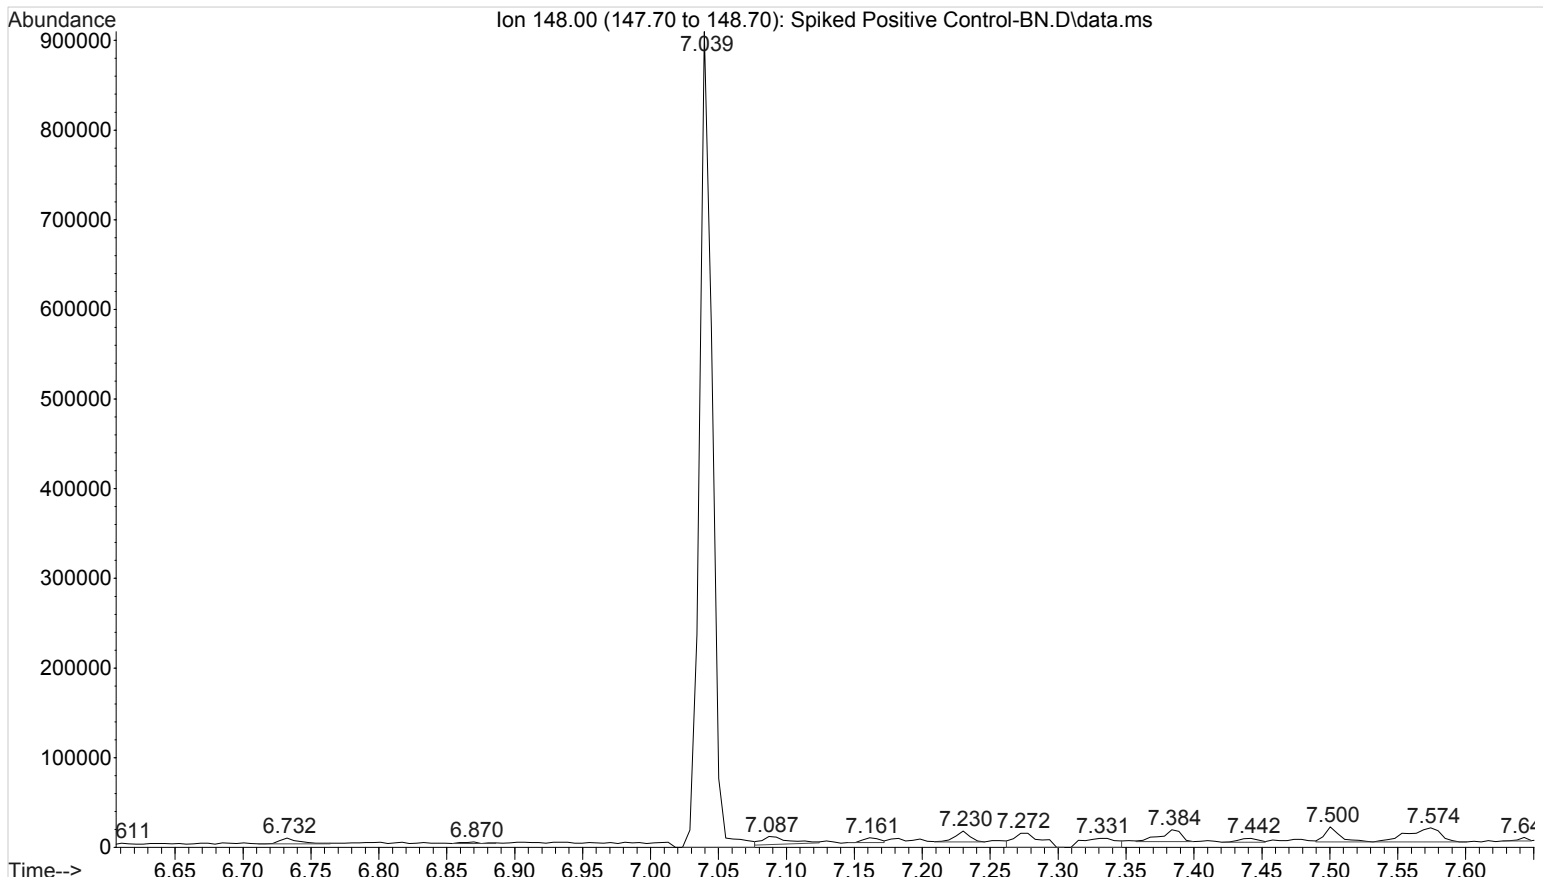



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\080516  
... \Spiked Positive Control-BN.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 05 Aug 2016 16:19 using AcqMethod BNSB120510.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

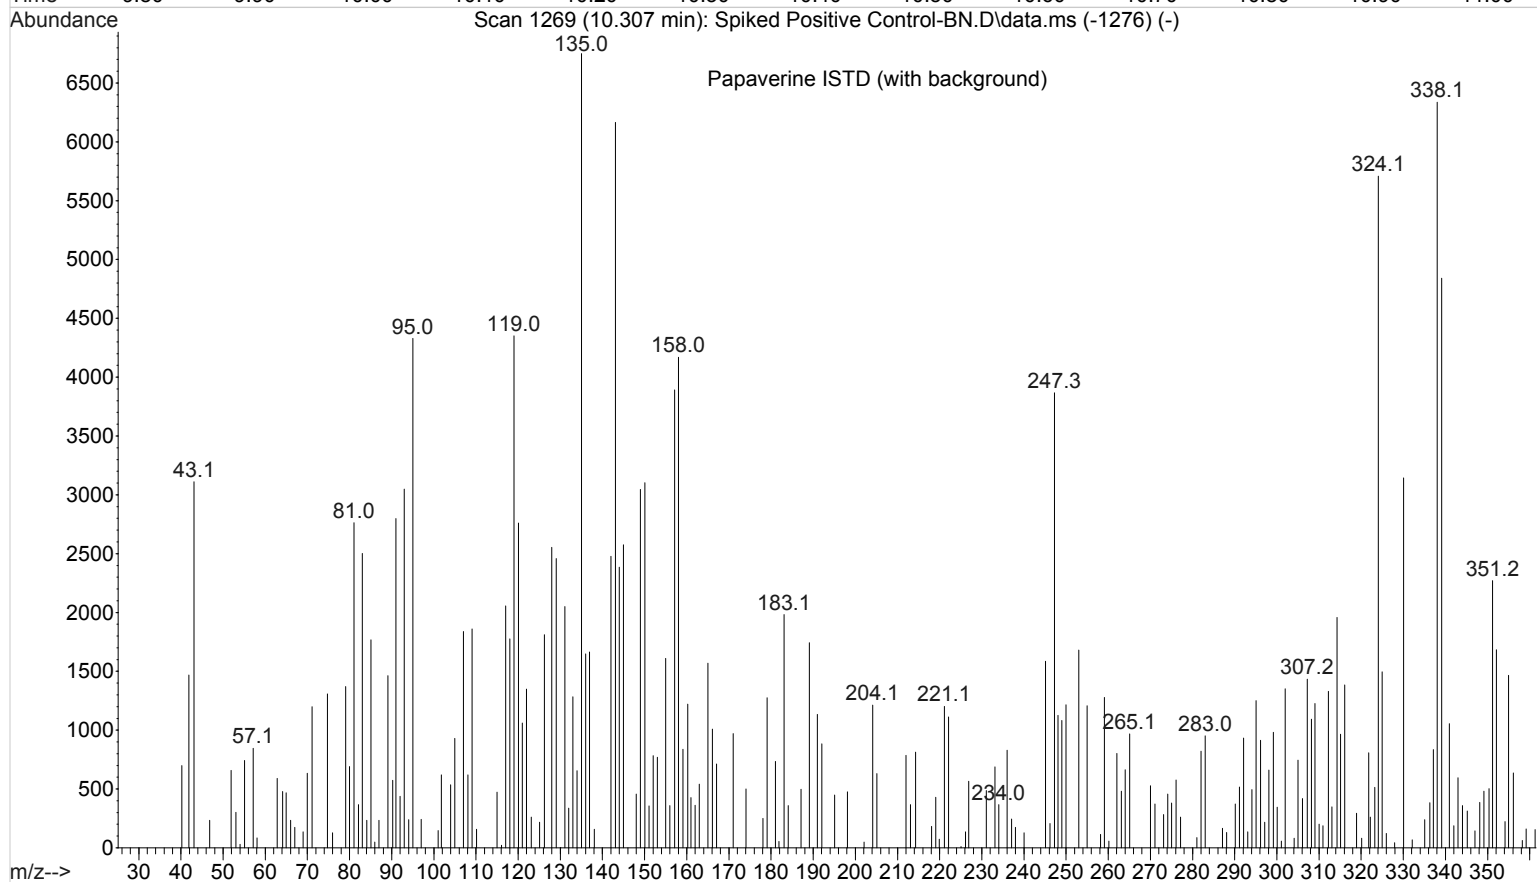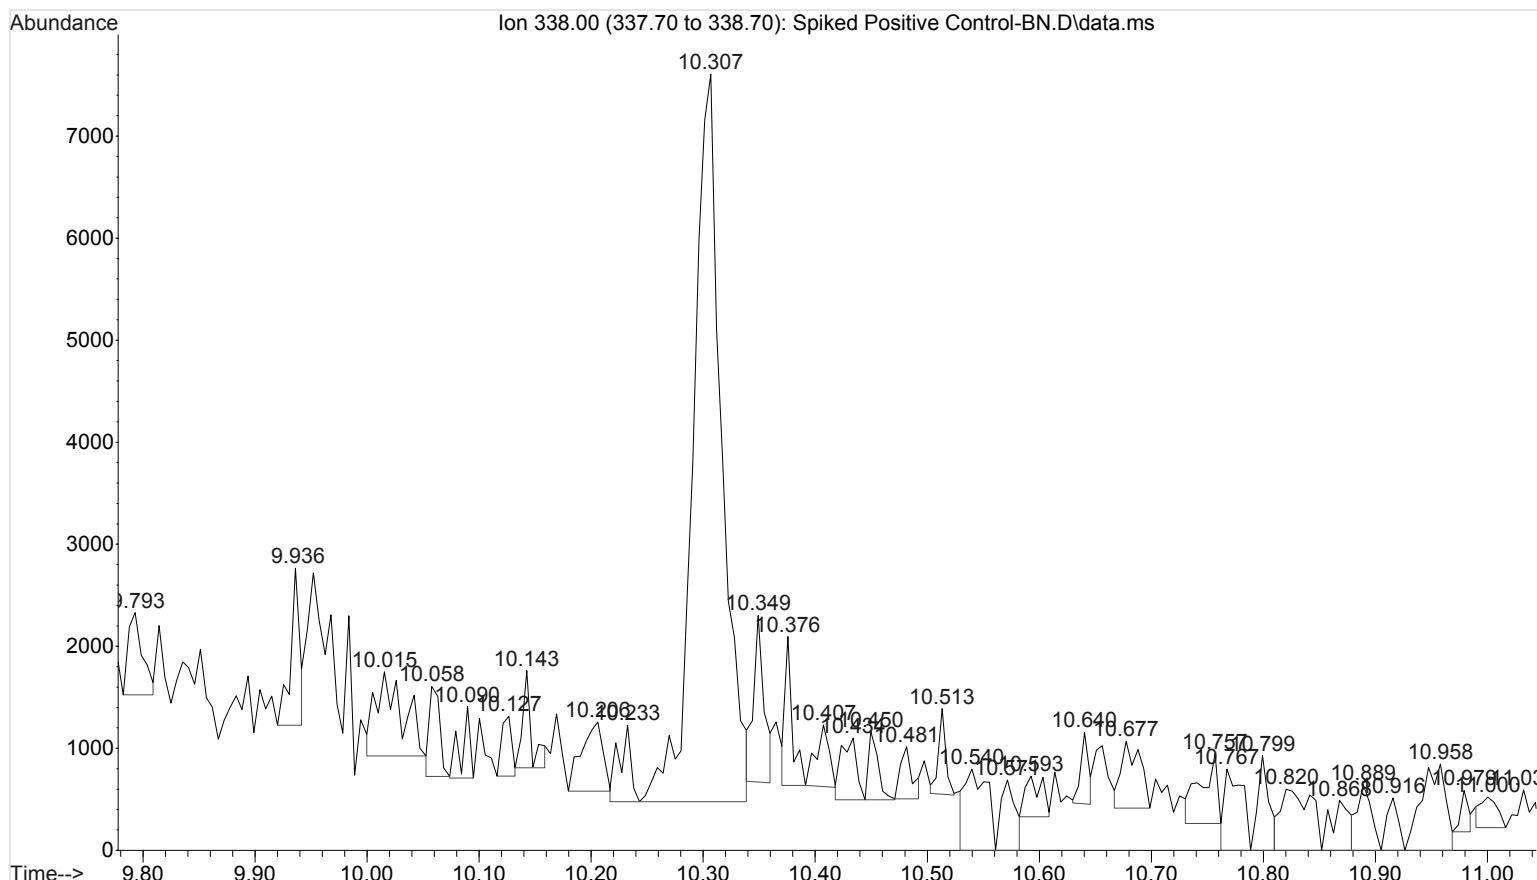



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\080516  
... \Spiked Positive Control-BN.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 05 Aug 2016 16:19 using AcqMethod BNSB120510.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

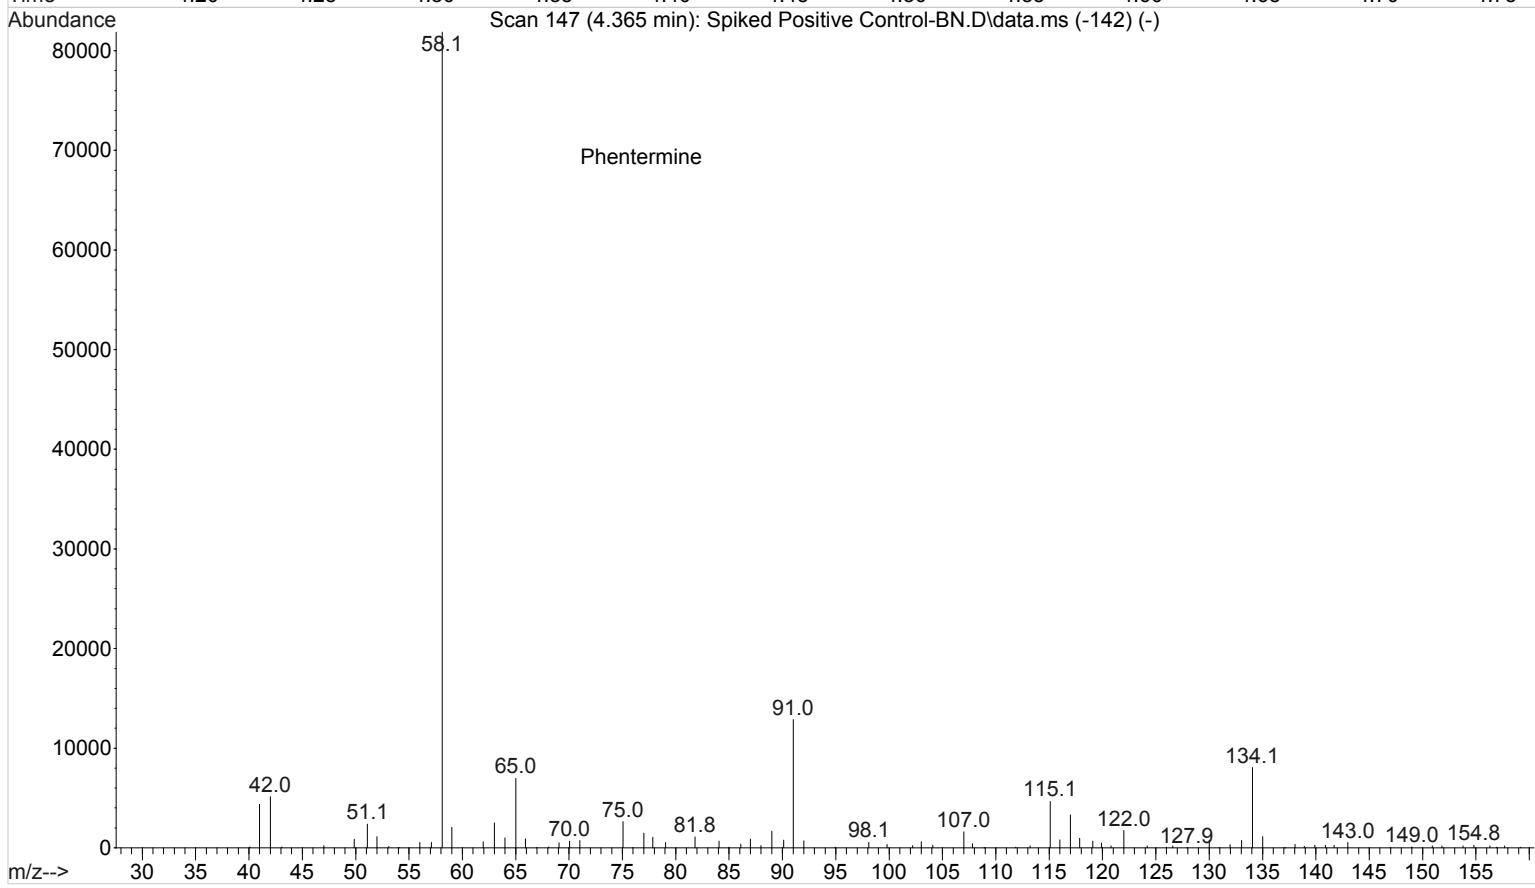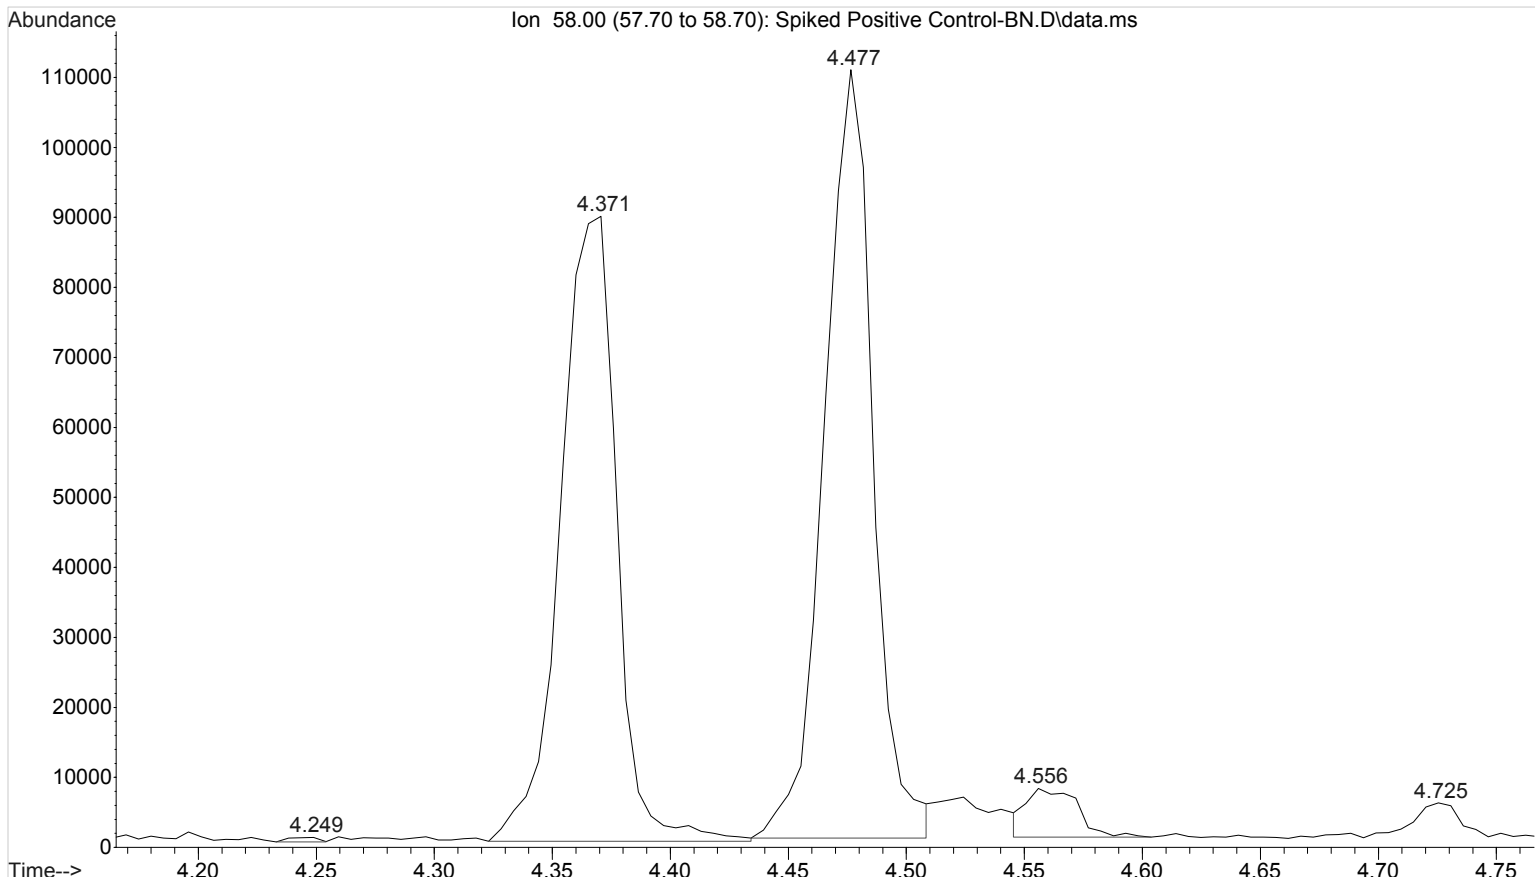



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\080516  
... \Spiked Positive Control-BN.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 05 Aug 2016 16:19 using AcqMethod BNSB120510.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

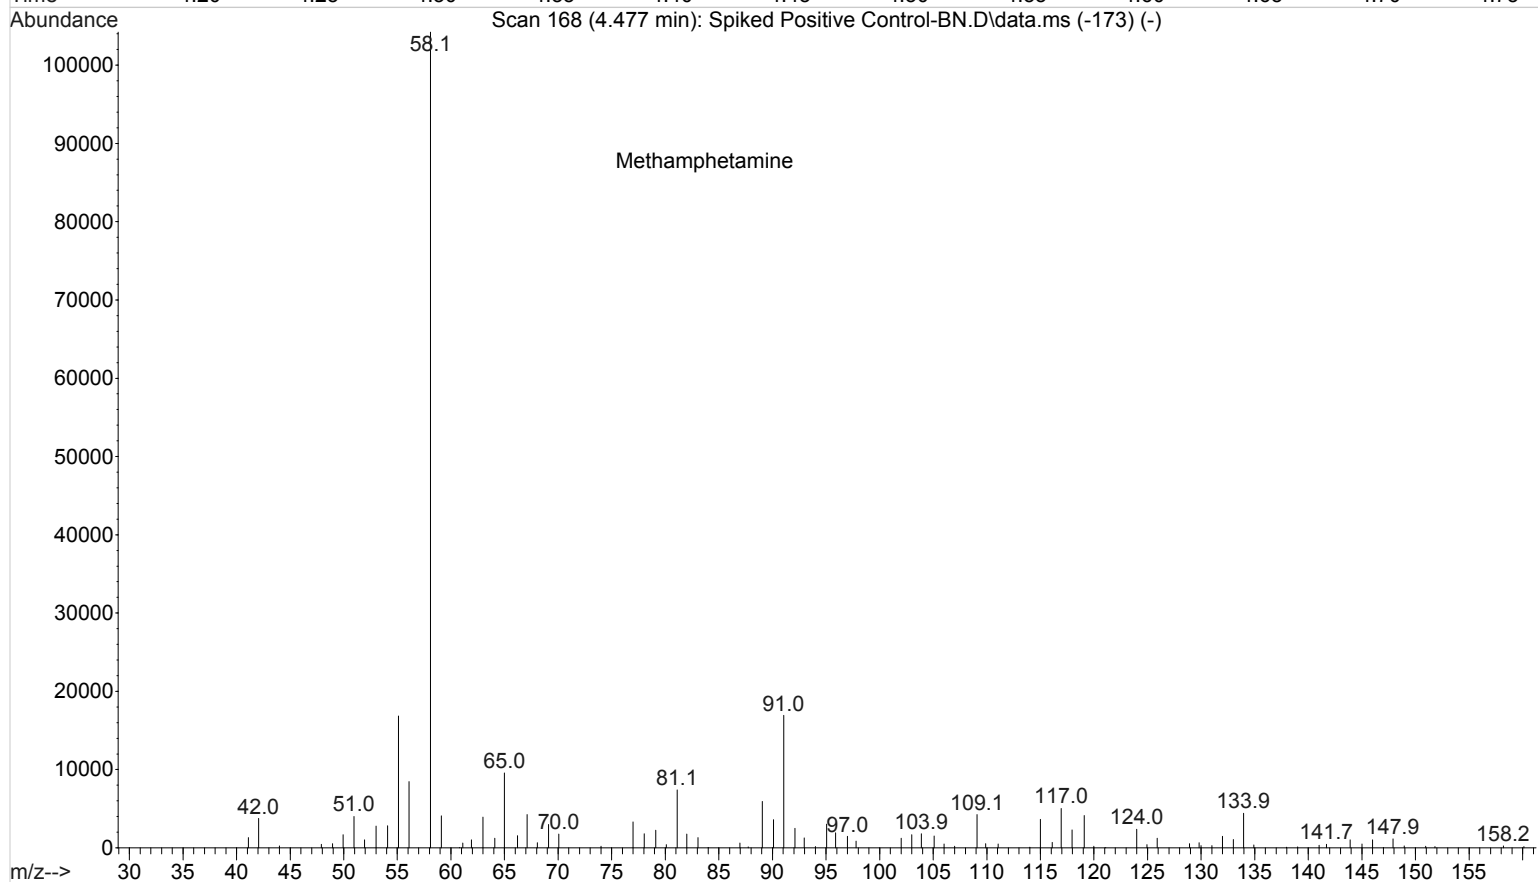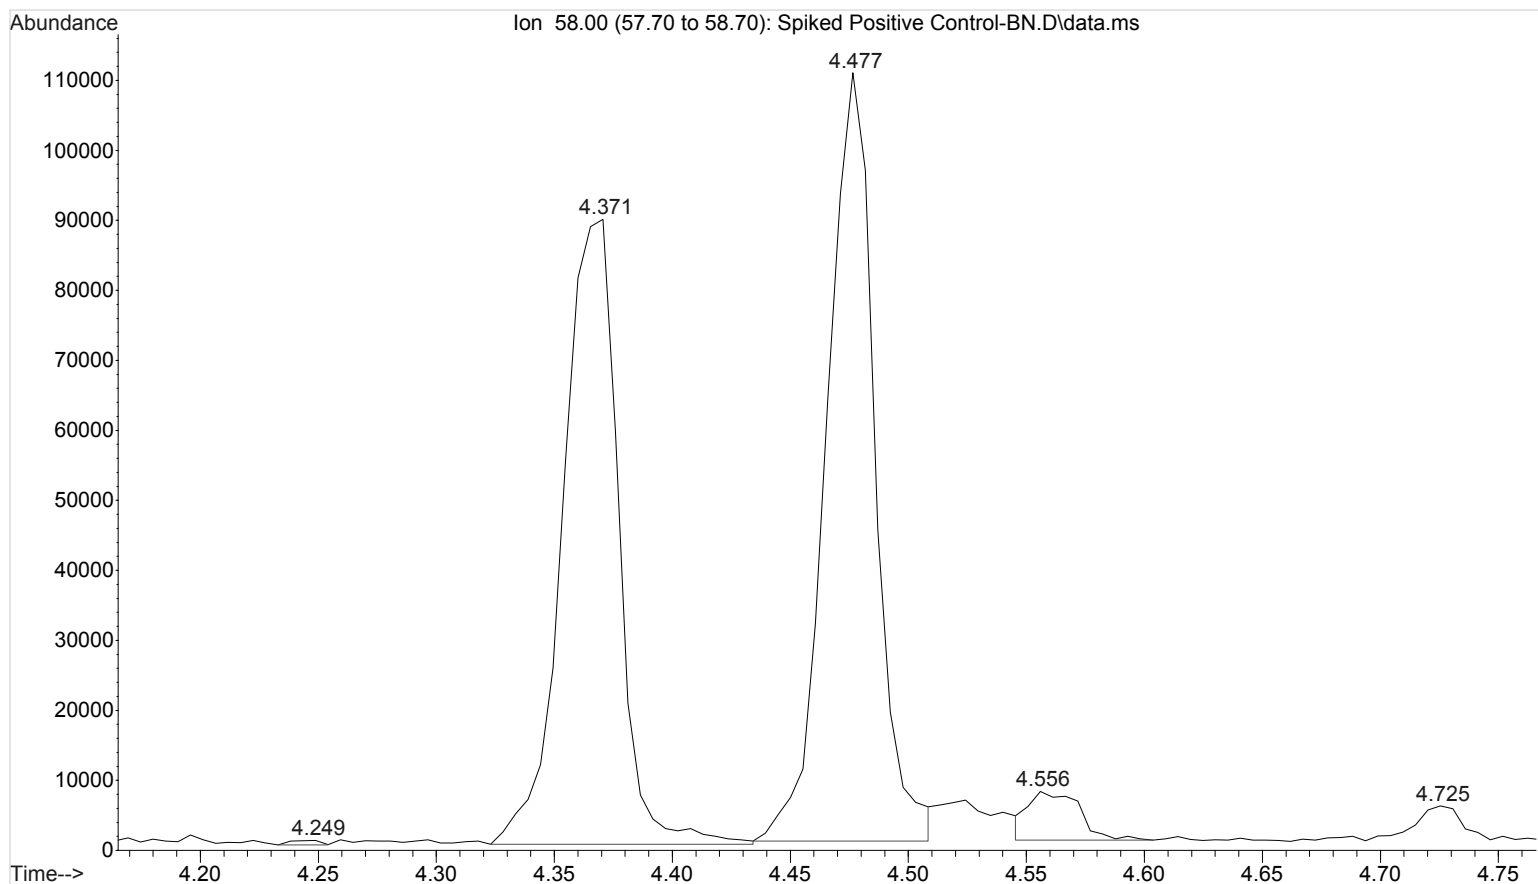

File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\080516  
... \Spiked Positive Control-BN.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 05 Aug 2016 16:19 using AcqMethod BNSB120510.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

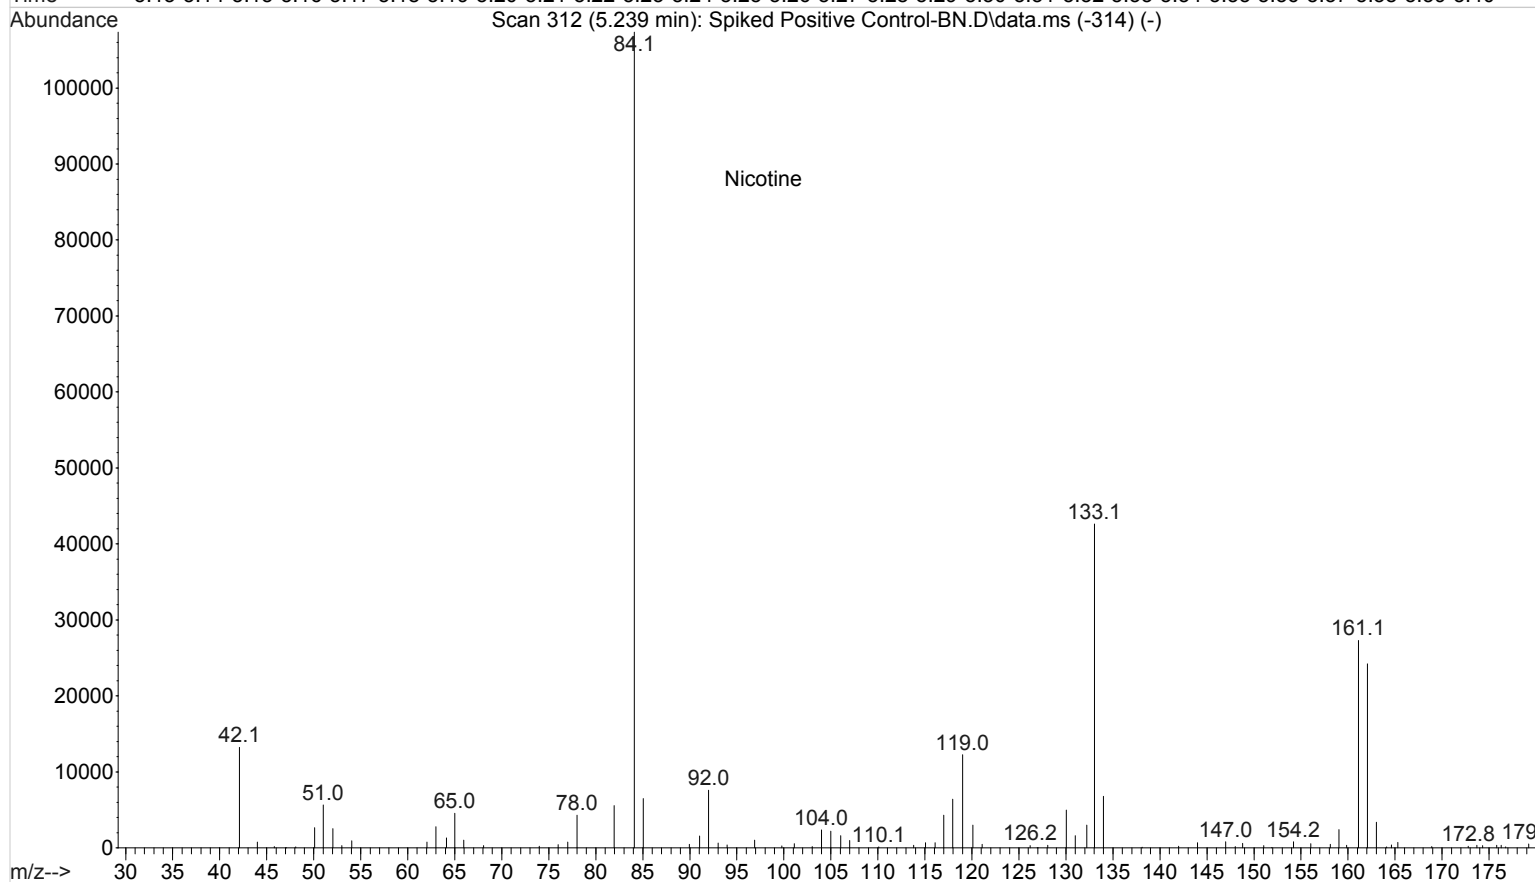
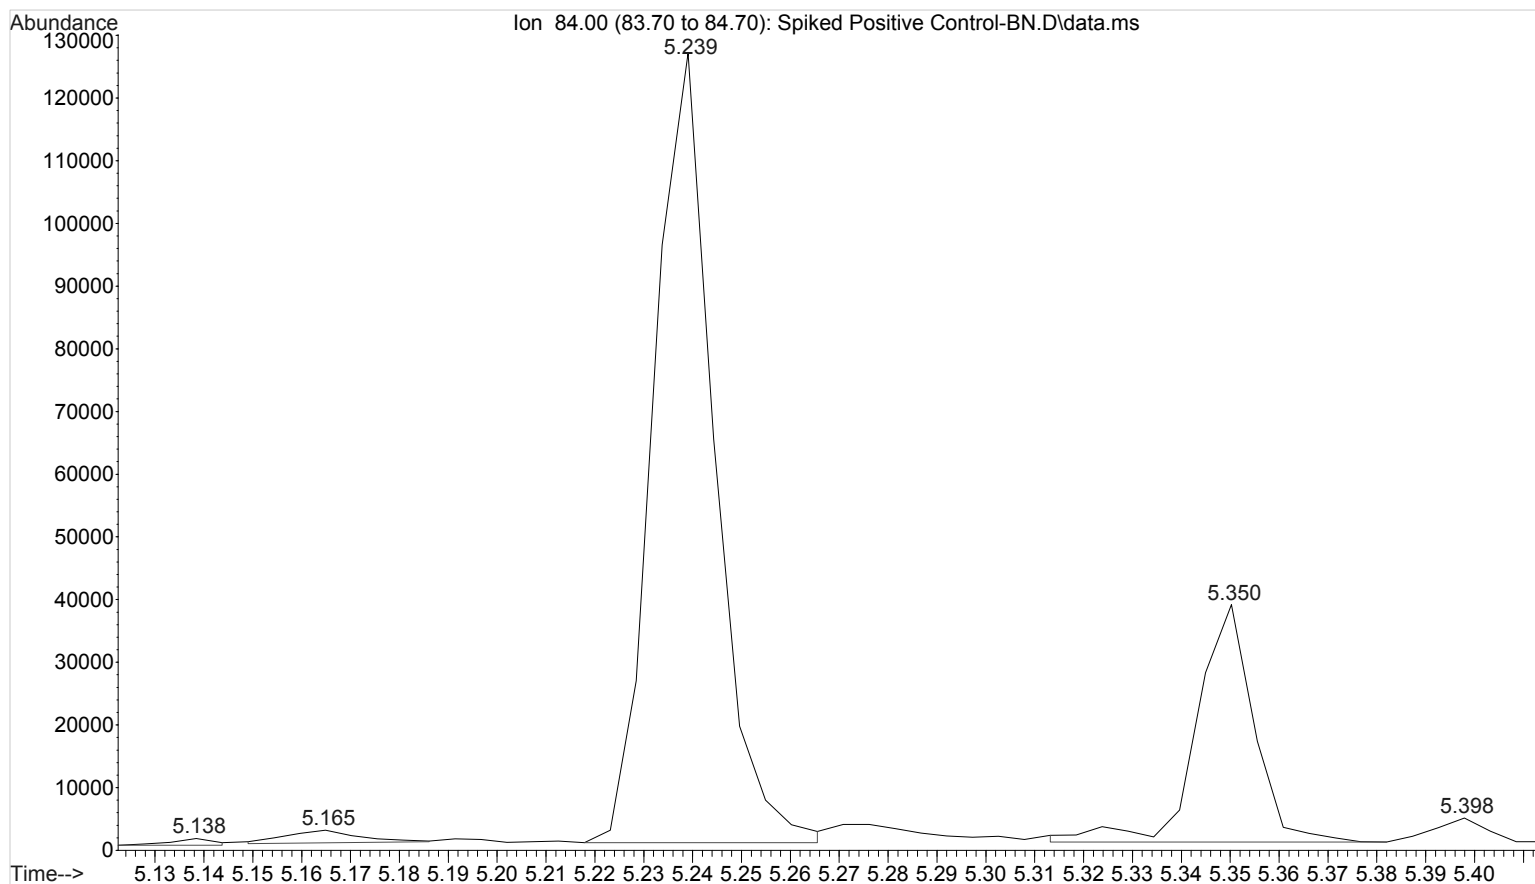


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\080516  
... \Spiked Positive Control-BN.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 05 Aug 2016 16:19 using AcqMethod BNSB120510.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

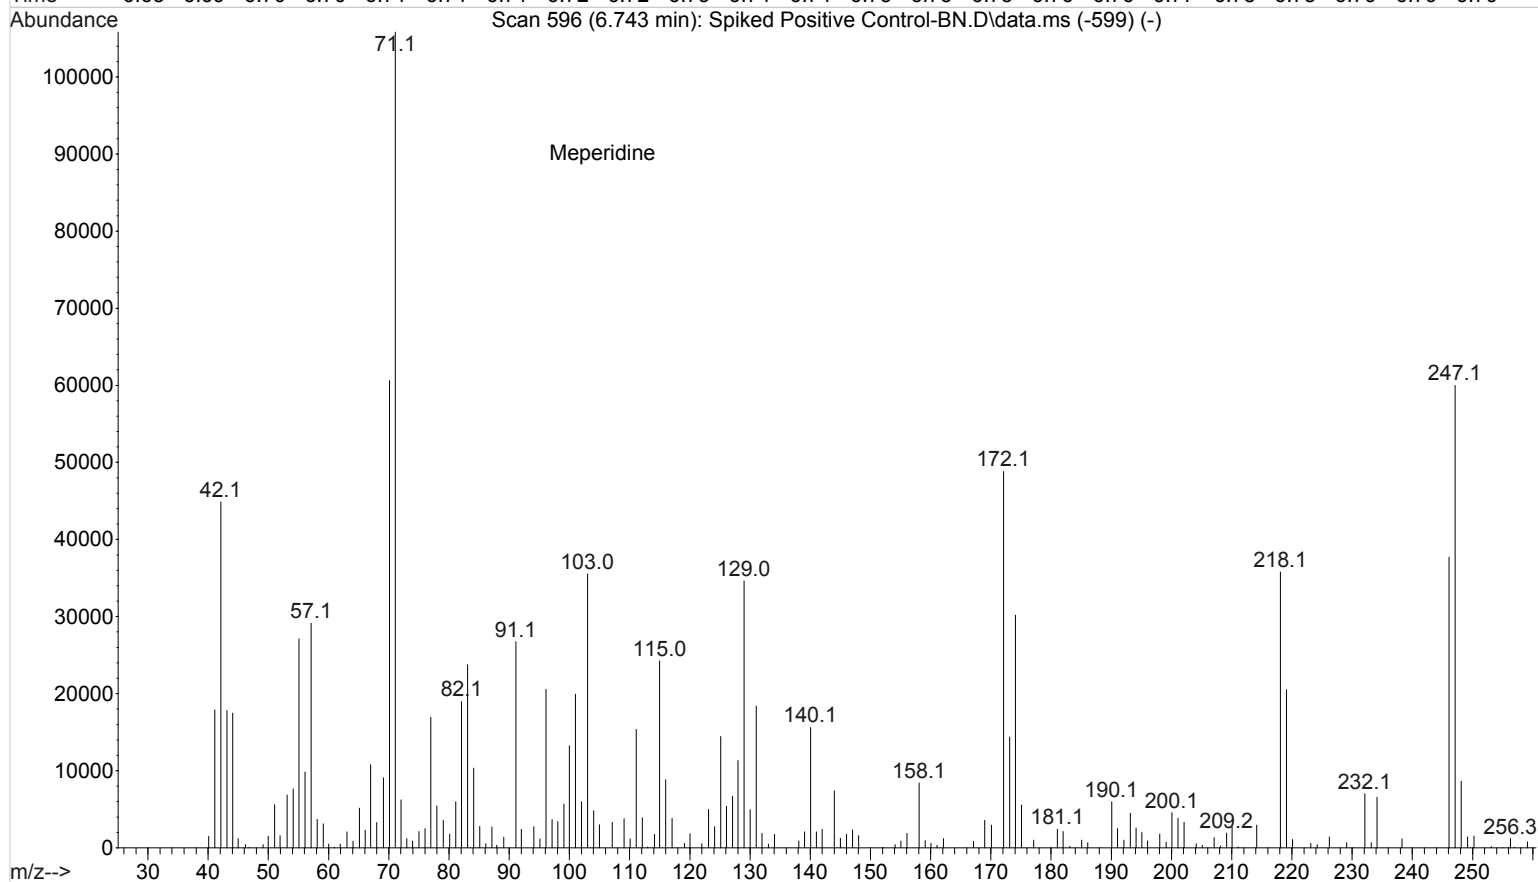
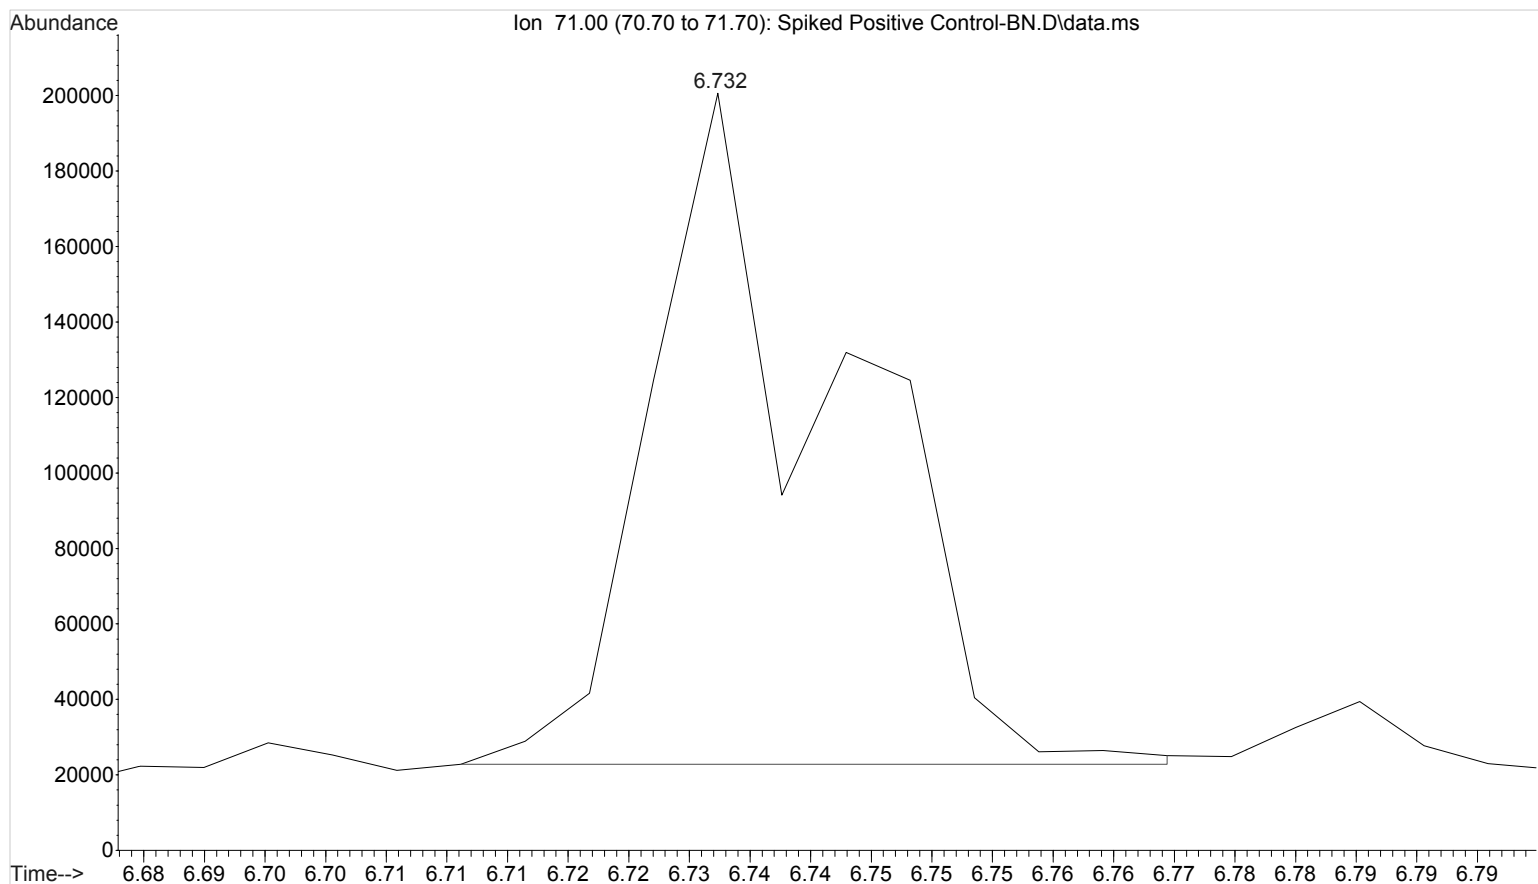






File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\080516  
... \Spiked Positive Control-BN.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 05 Aug 2016 16:19 using AcqMethod BNSB120510.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

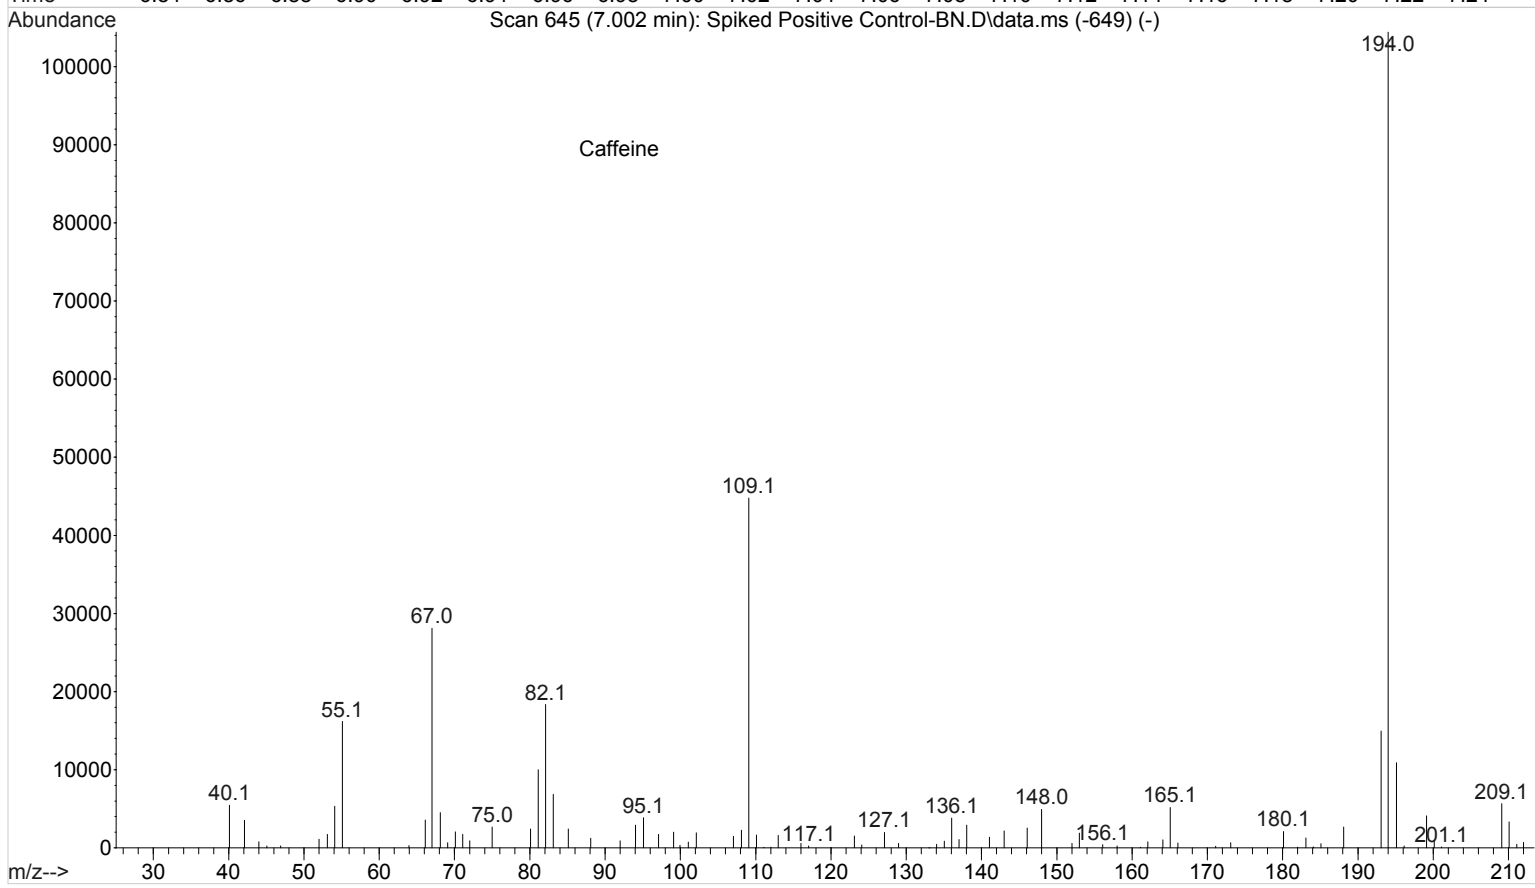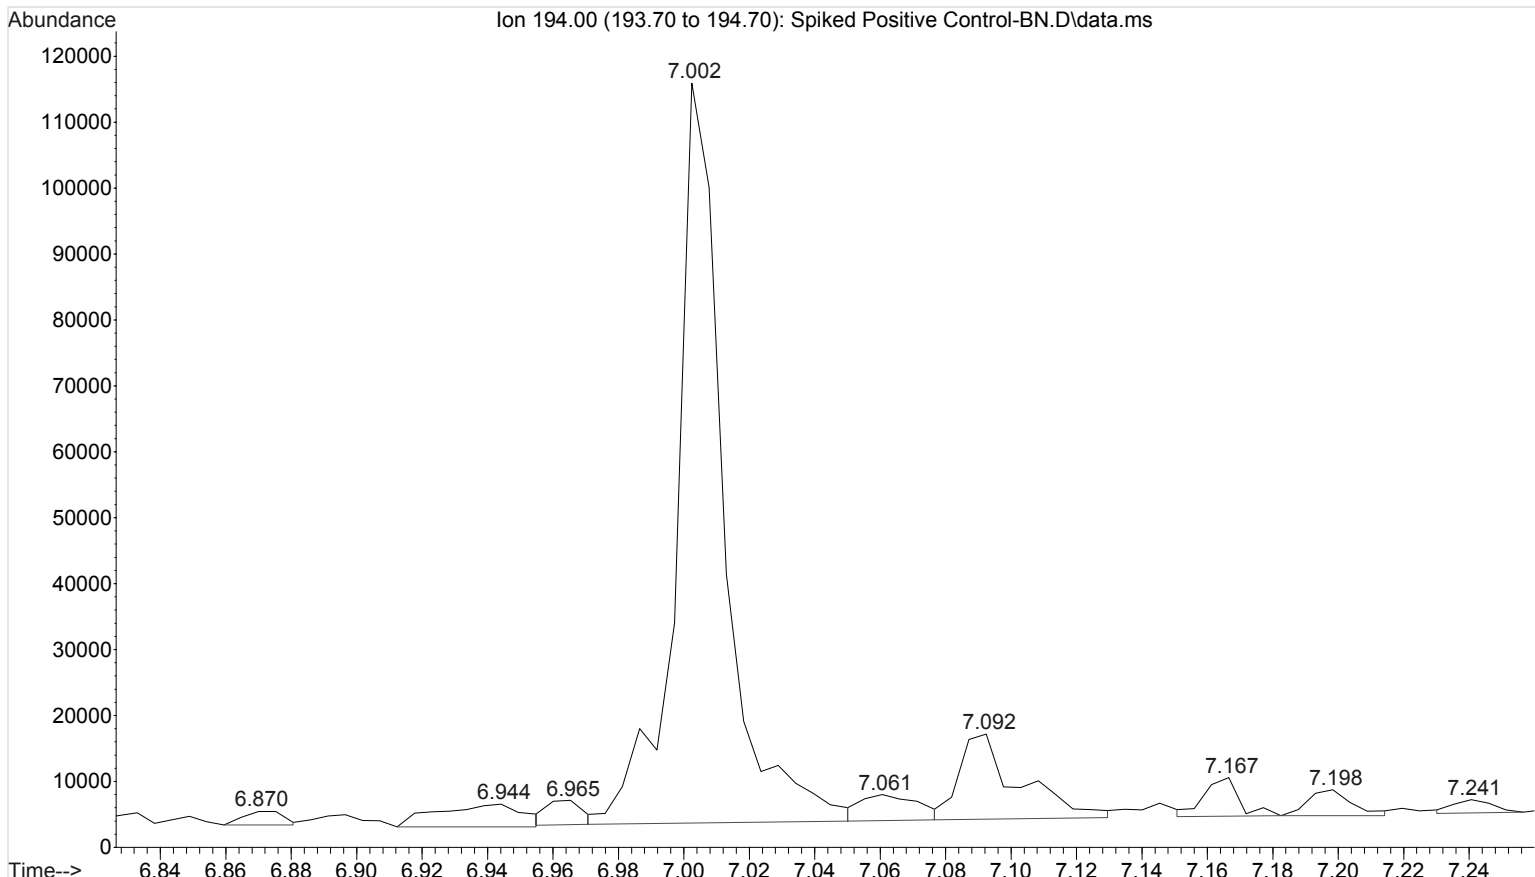

File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\080516  
... \Spiked Positive Control-BN.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 05 Aug 2016 16:19 using AcqMethod BNSB120510.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

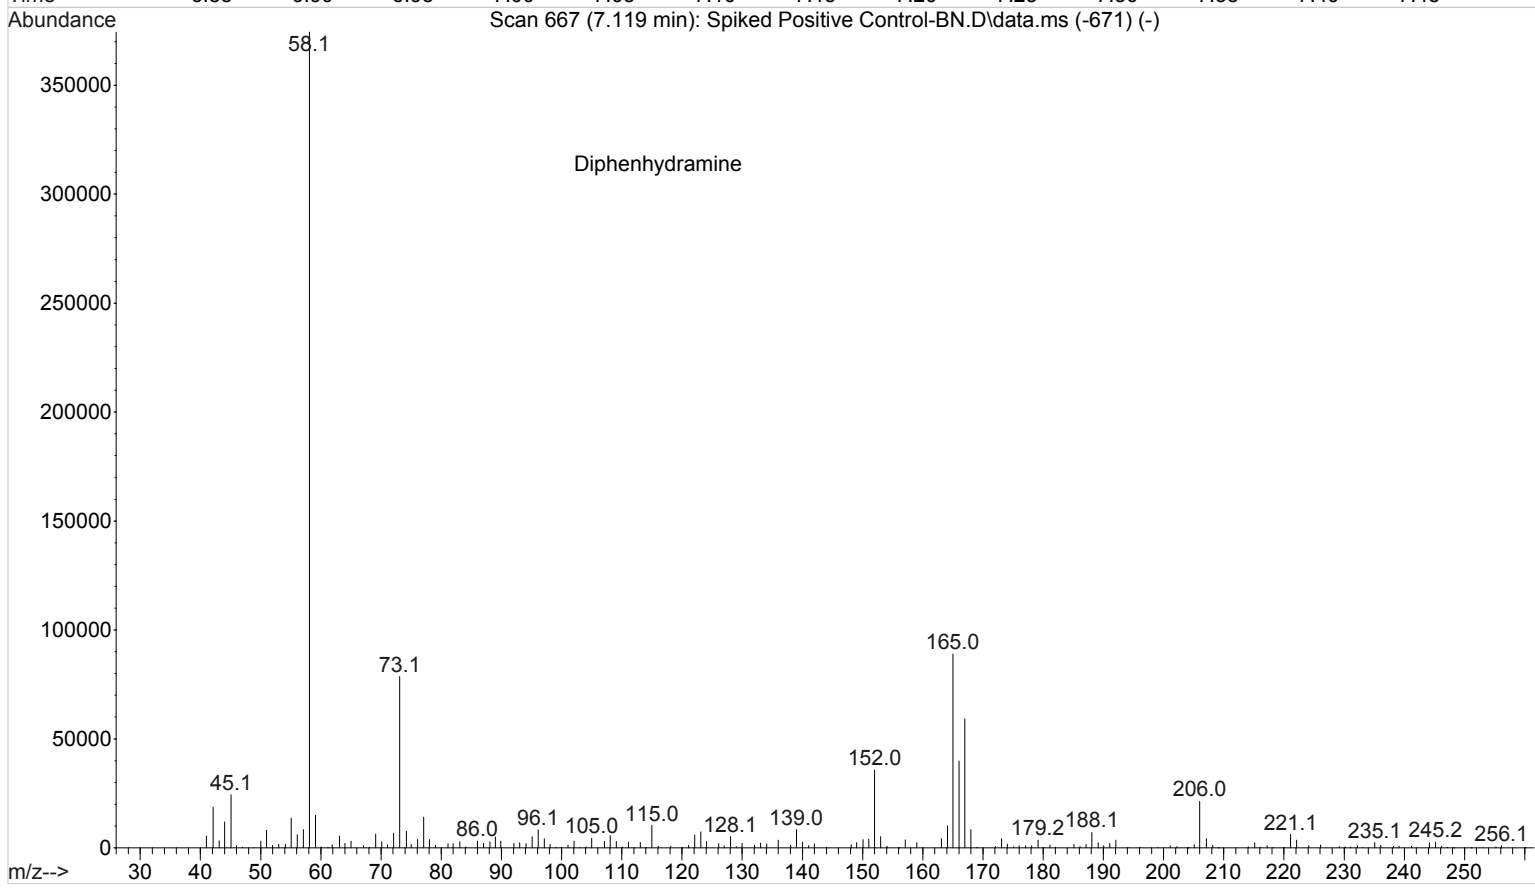
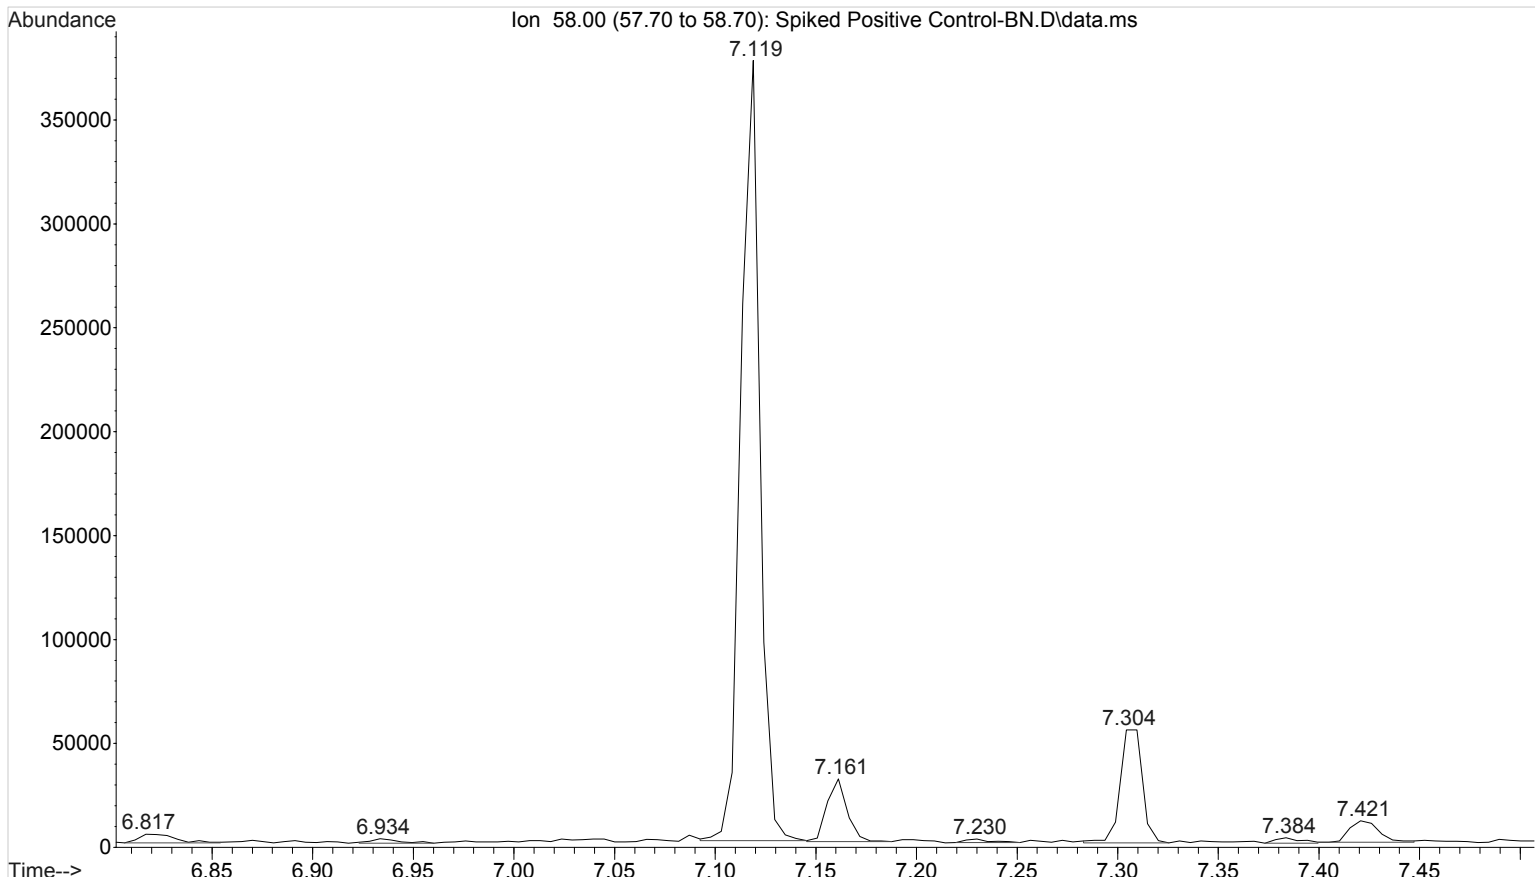


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\080516  
... \Spiked Positive Control-BN.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 05 Aug 2016 16:19 using AcqMethod BNSB120510.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

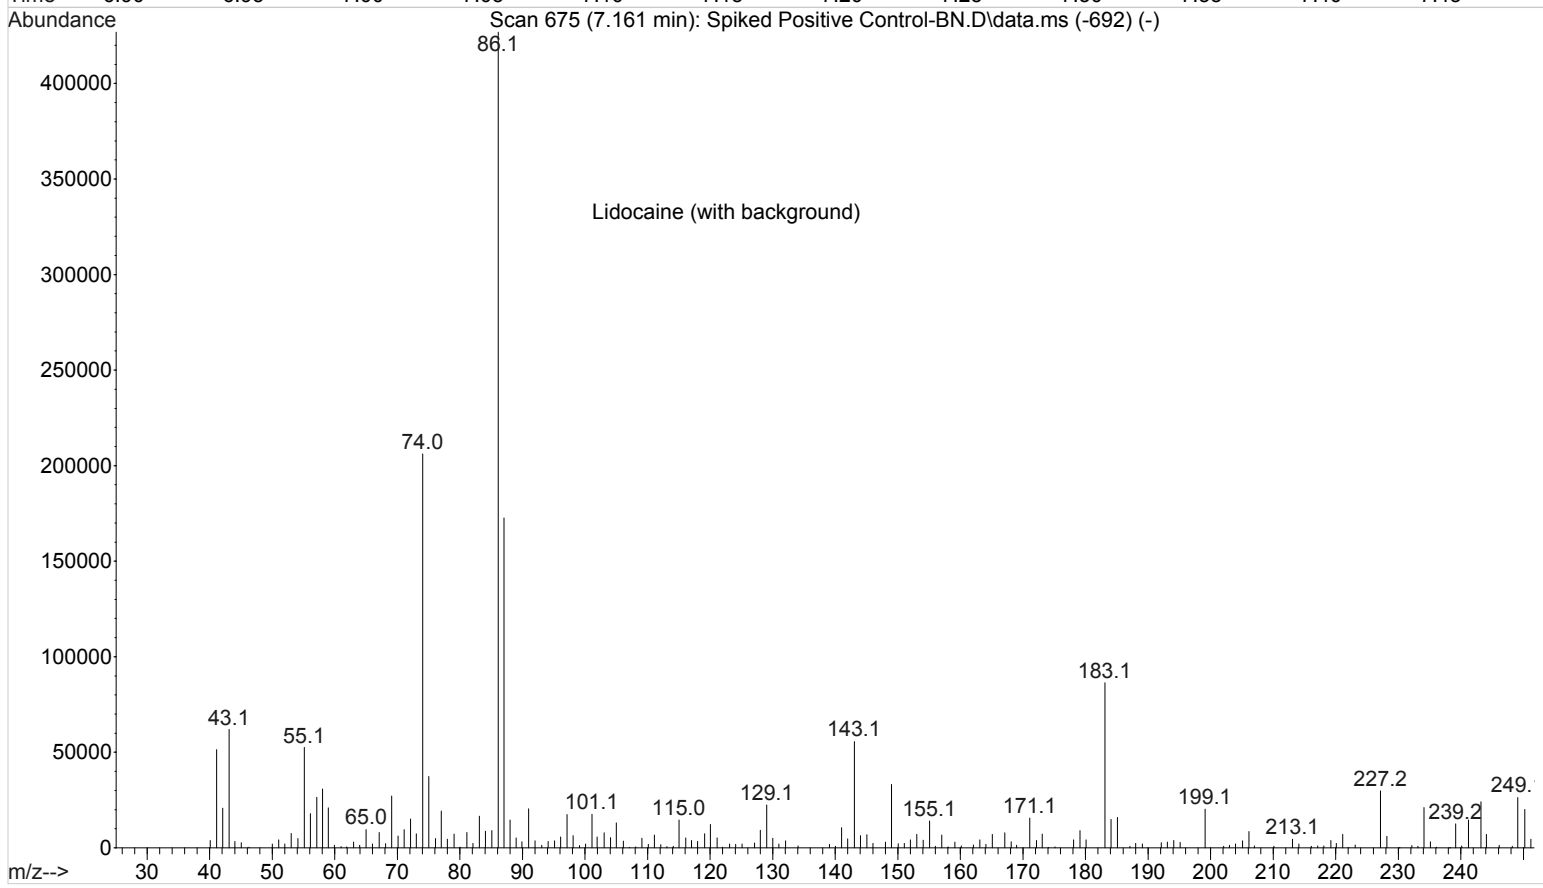
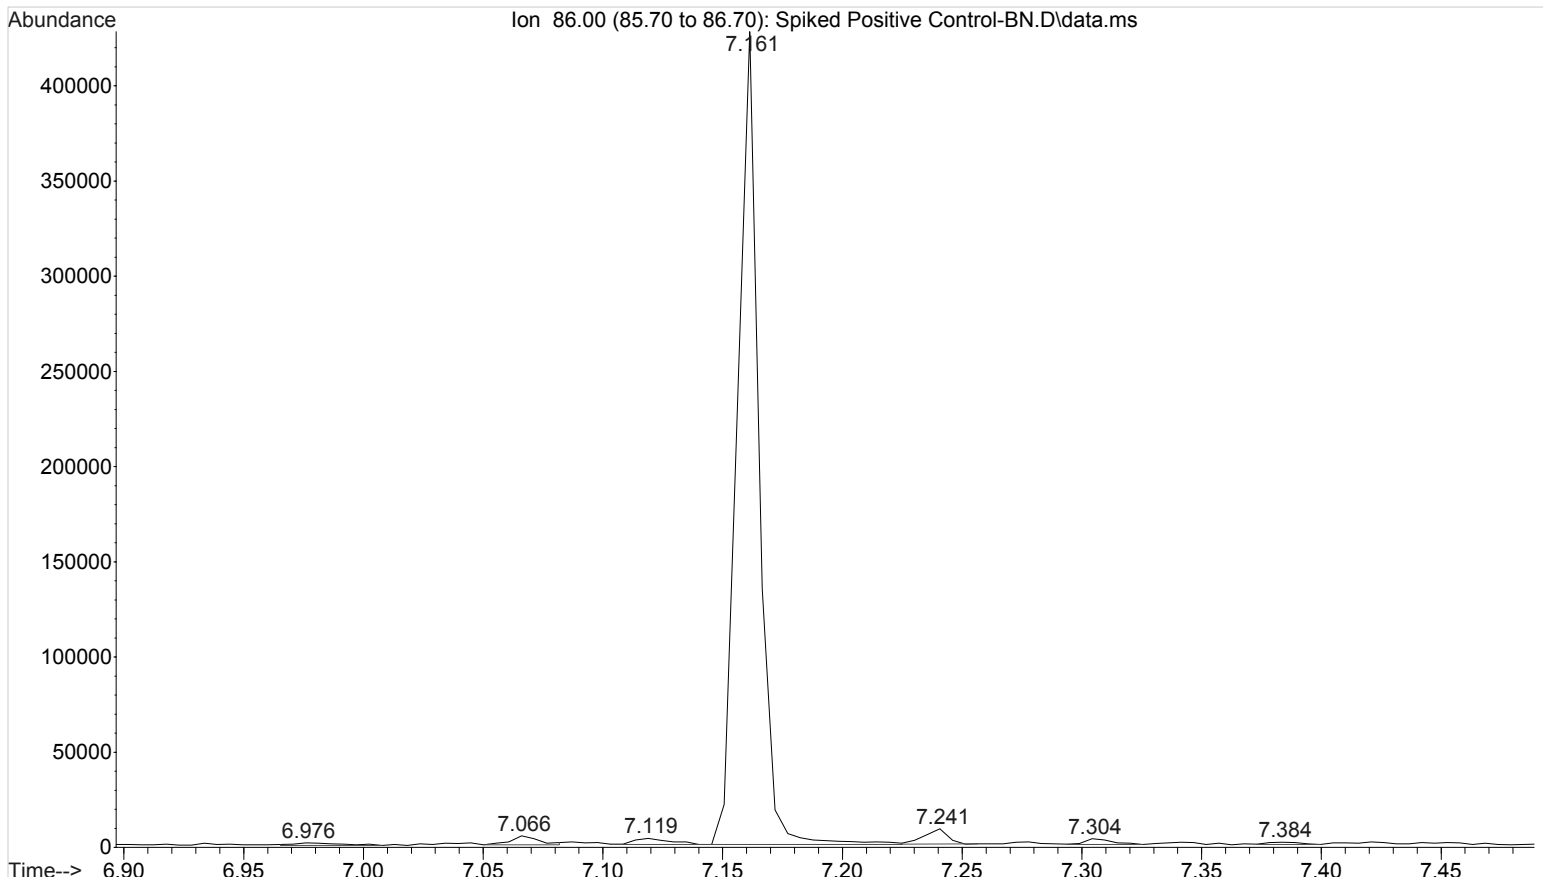


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\080516  
... \Spiked Positive Control-BN.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 05 Aug 2016 16:19 using AcqMethod BNSB120510.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215



9

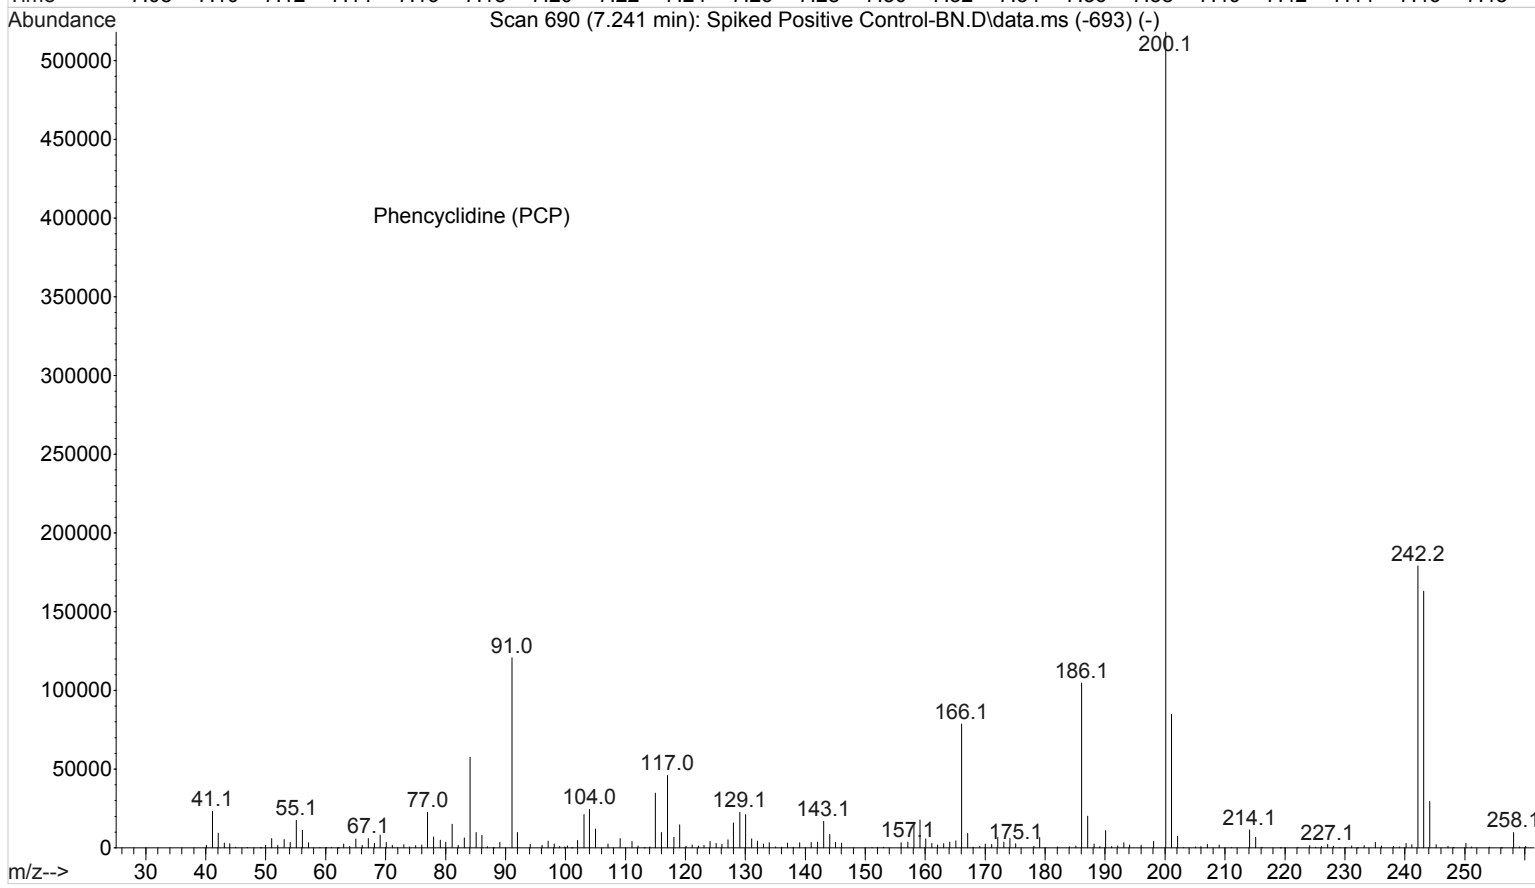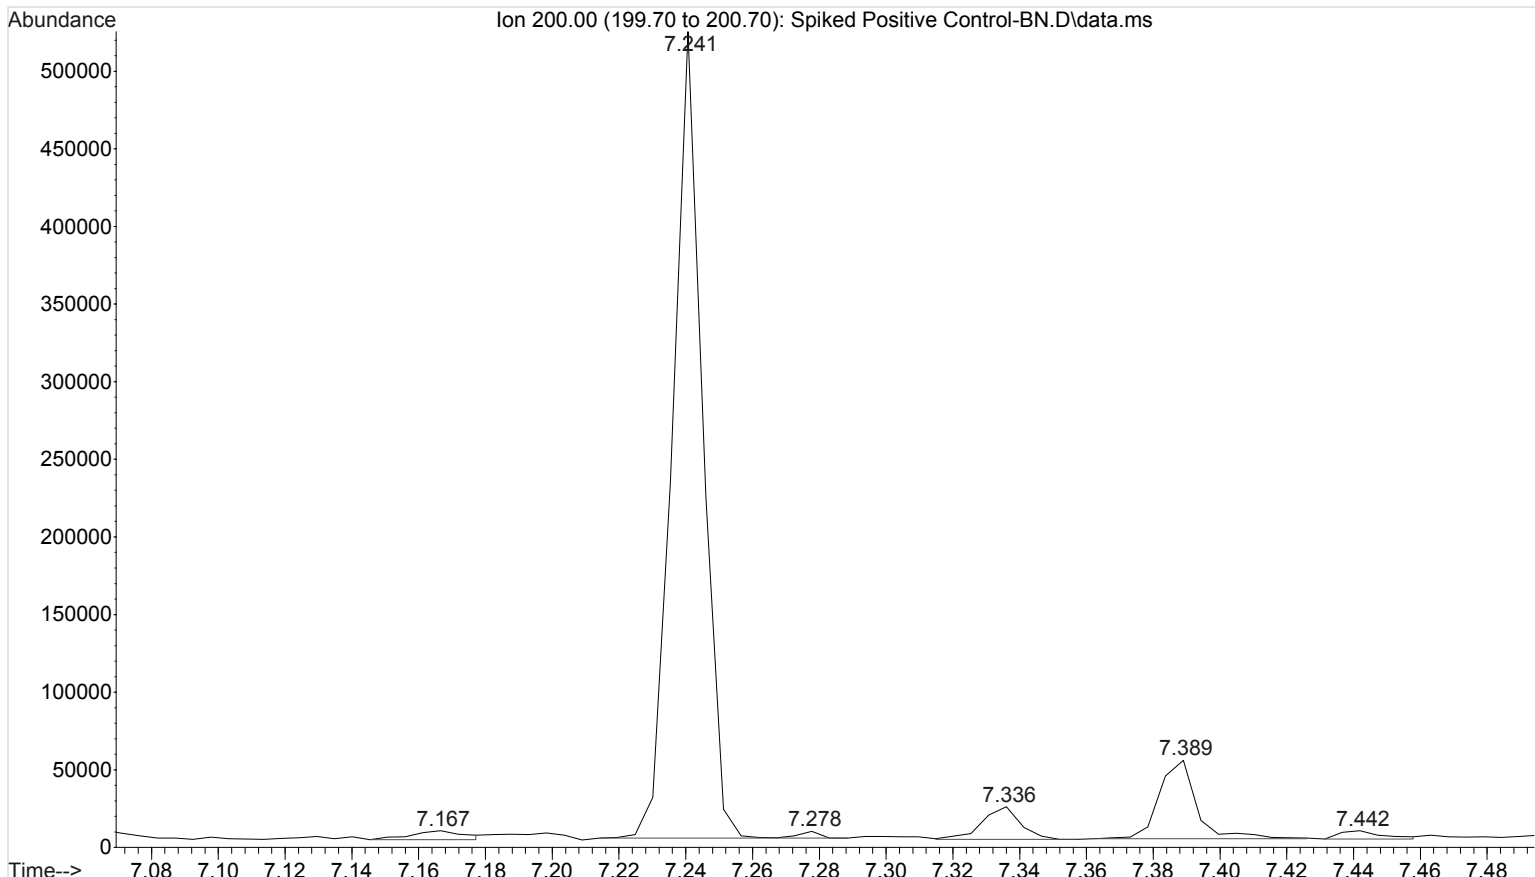

File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\080516  
... \Spiked Positive Control-BN.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 05 Aug 2016 16:19 using AcqMethod BNSB120510.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

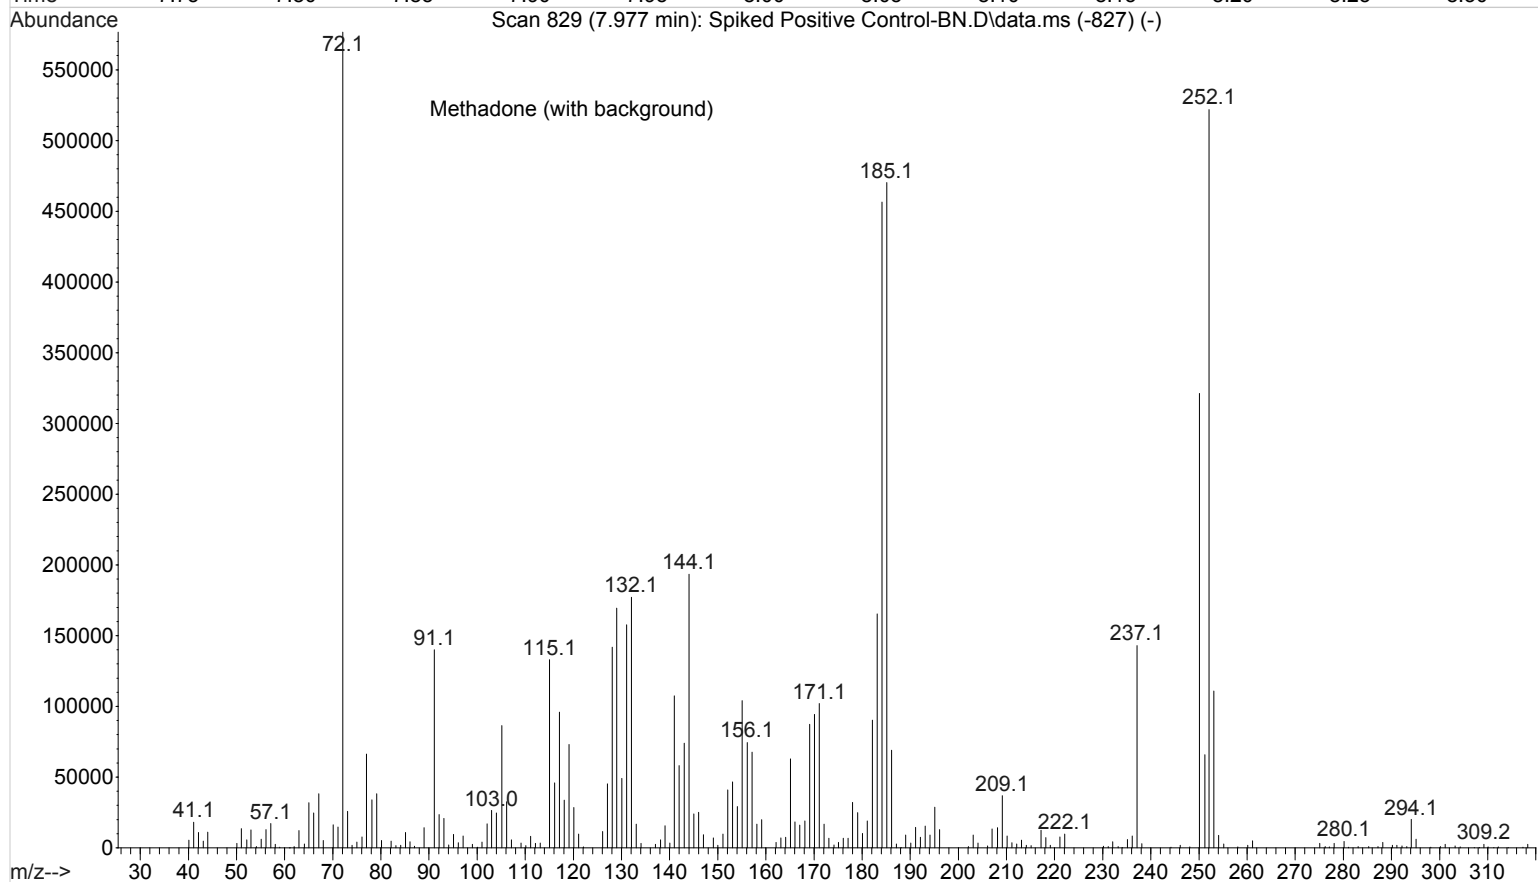
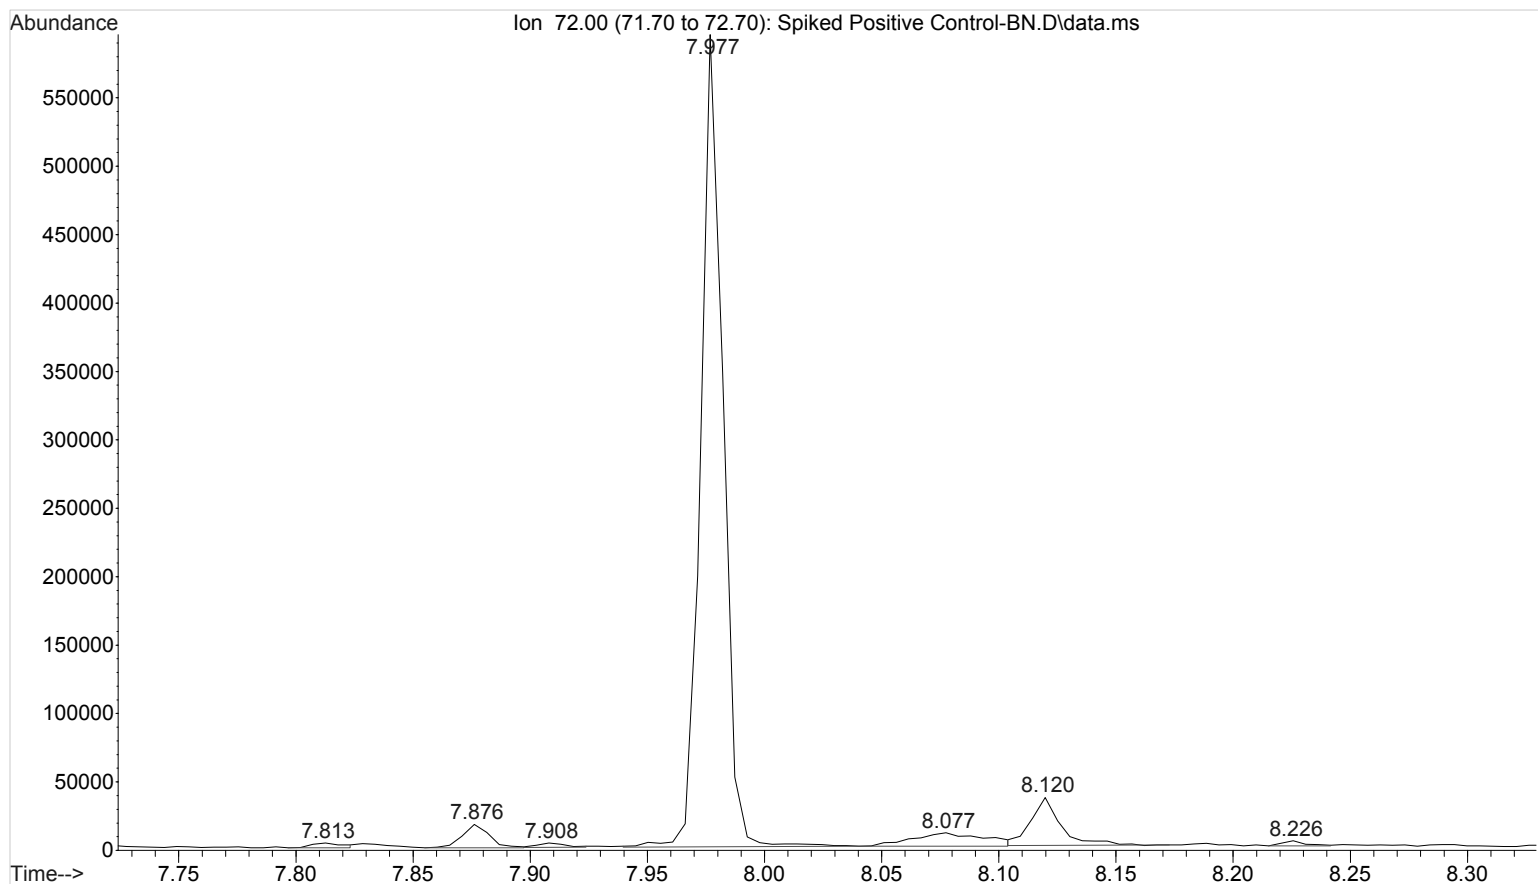


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\080516  
... \Spiked Positive Control-BN.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 05 Aug 2016 16:19 using AcqMethod BNSB120510.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

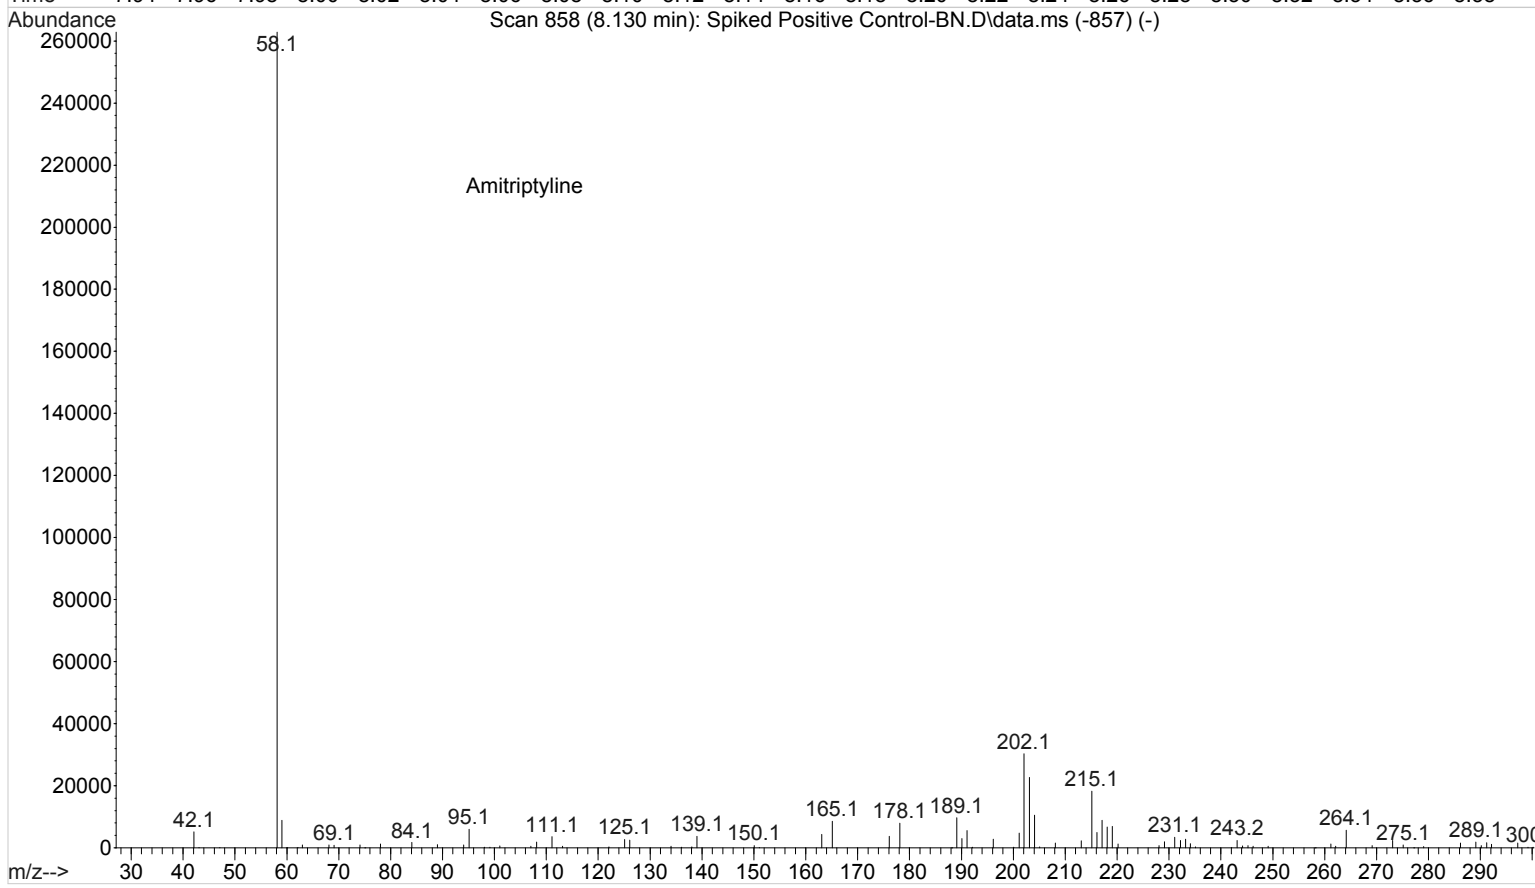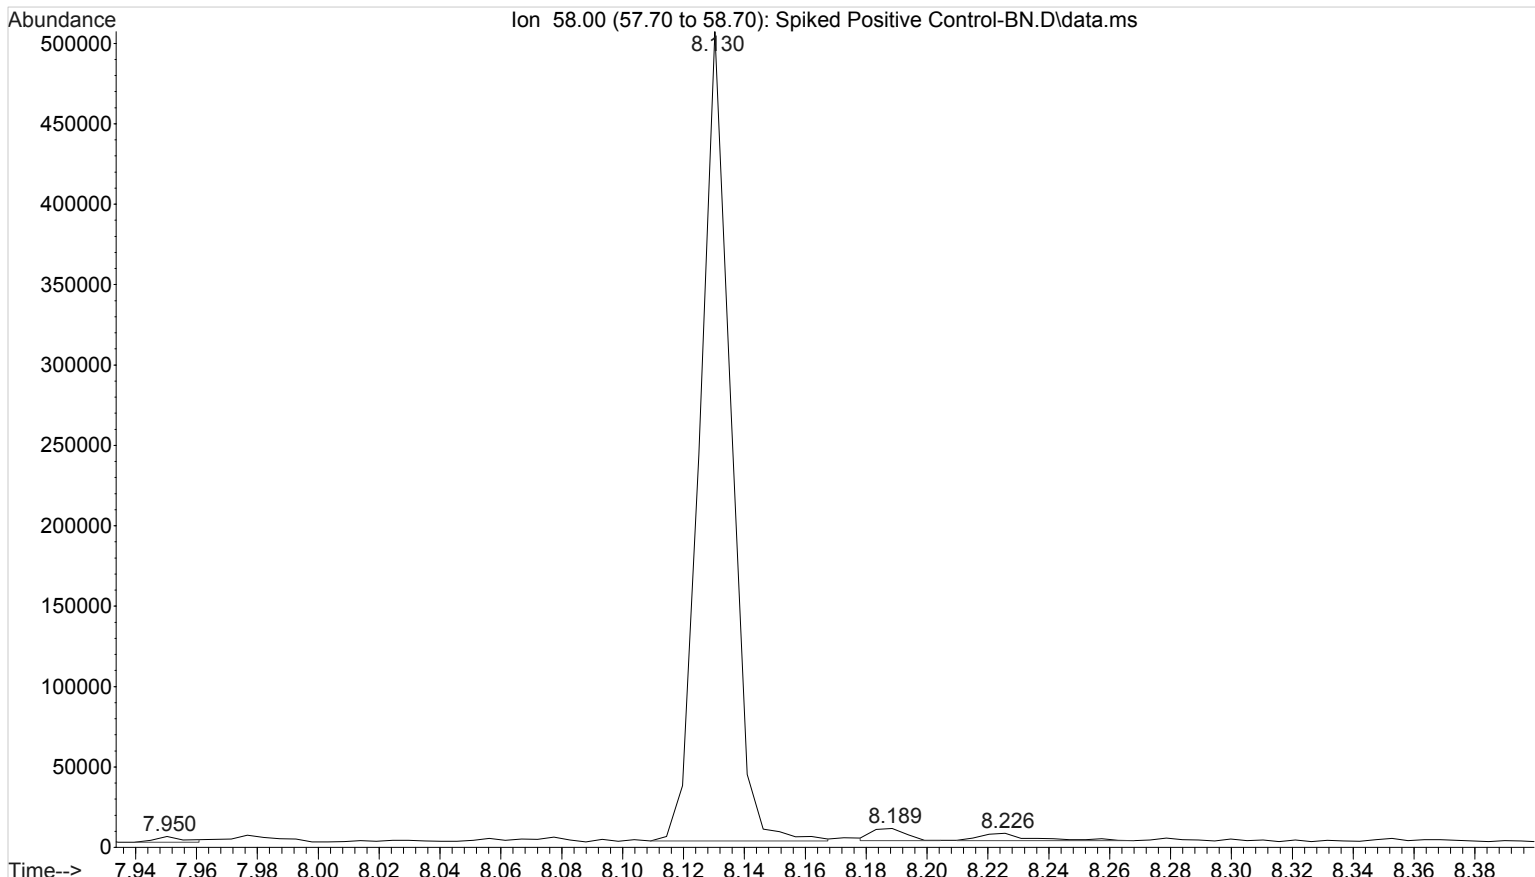

File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\080516  
... \Spiked Positive Control-BN.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 05 Aug 2016 16:19 using AcqMethod BNSB120510.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

9

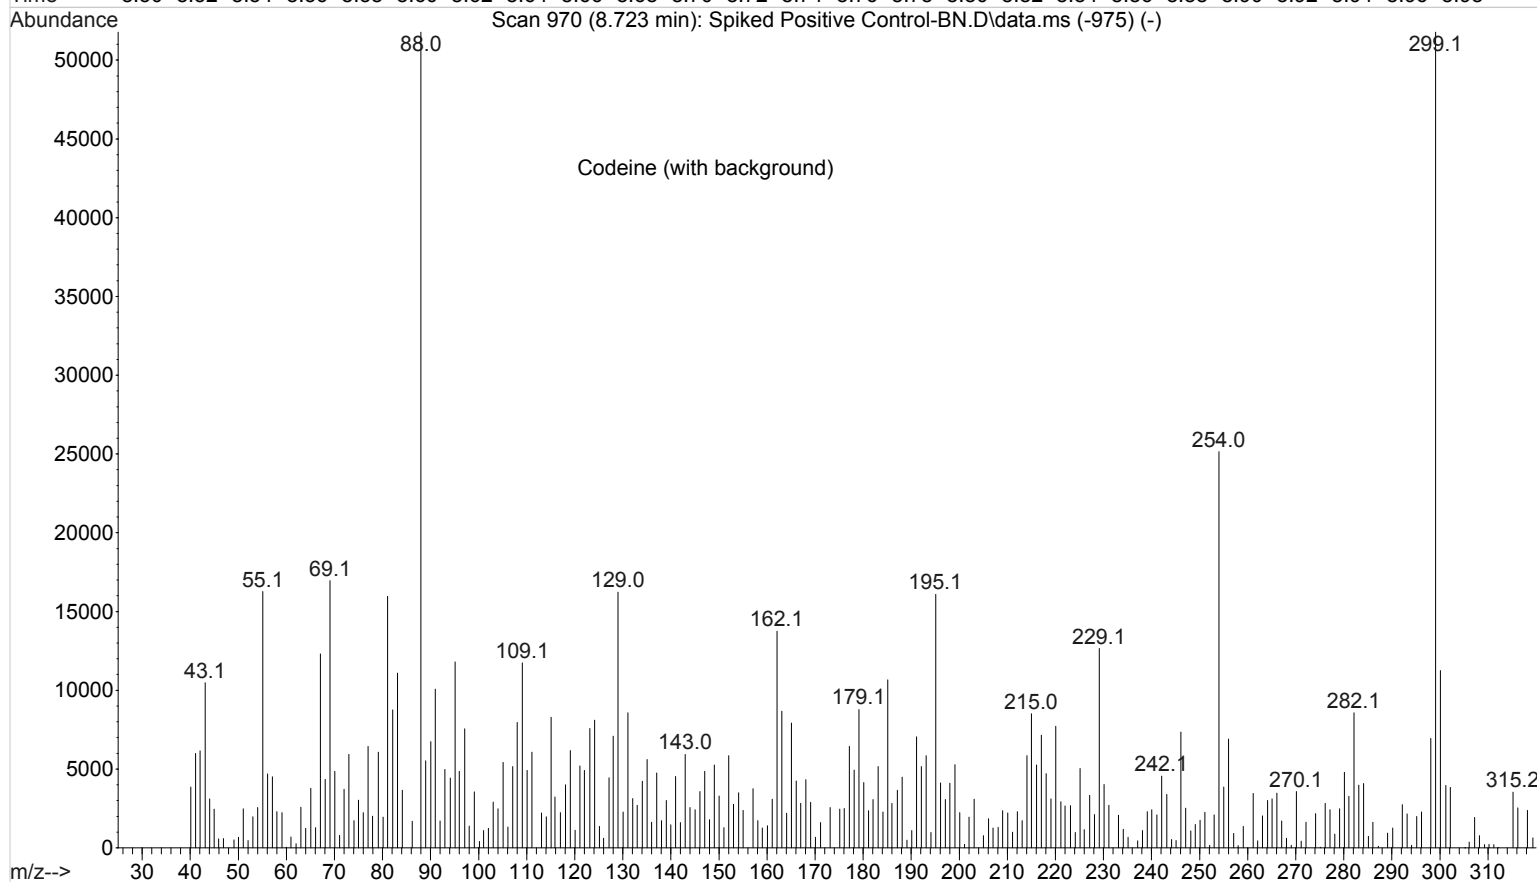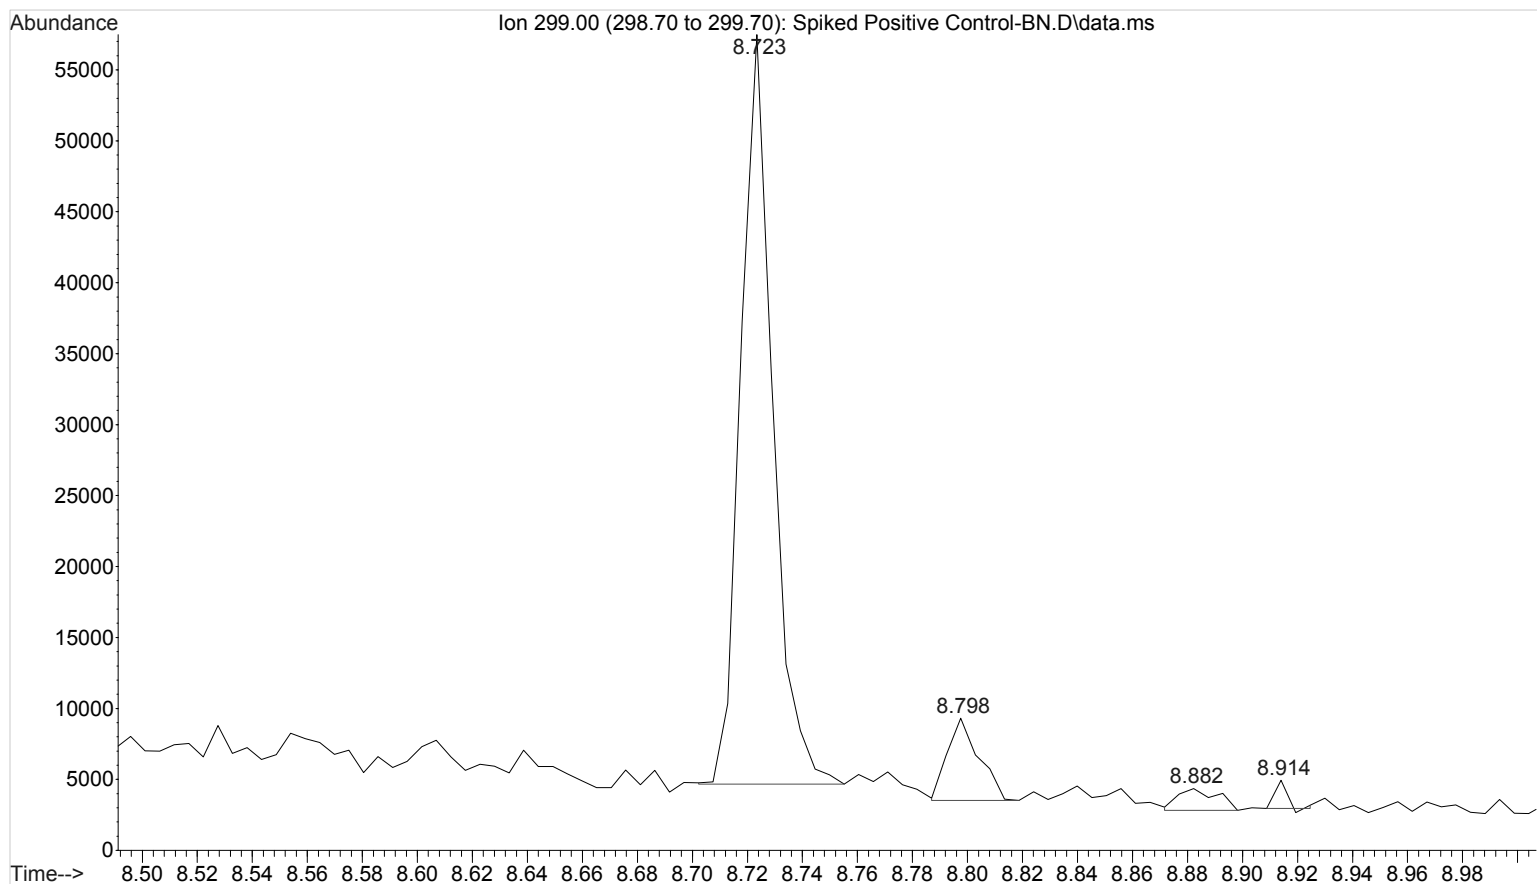

Analytical Method 3.6.1 & 3.6.7 QA Check List

---

Run Start Date: 08/05/2016

Analyst: CS

(Long GC/MS temperature program)

Positive Control Compound List

- Phentermine
- Methamphetamine
- Nicotine
- Meperidine
- Caffeine
- Diphenhydramine
- Lidocaine
- PCP
- Methadone
- Amitriptyline
- Codeine


Internal Standards

- Benzphetamine
- Papaverine



Optional back extraction **not** performed.  
Reconstituted in MeOH.





File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\080516  
... \Negative Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 05 Aug 2016 17:39 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Negative Control - Utak Lot B1013  
Misc Info : Analytical Method 3.6.1

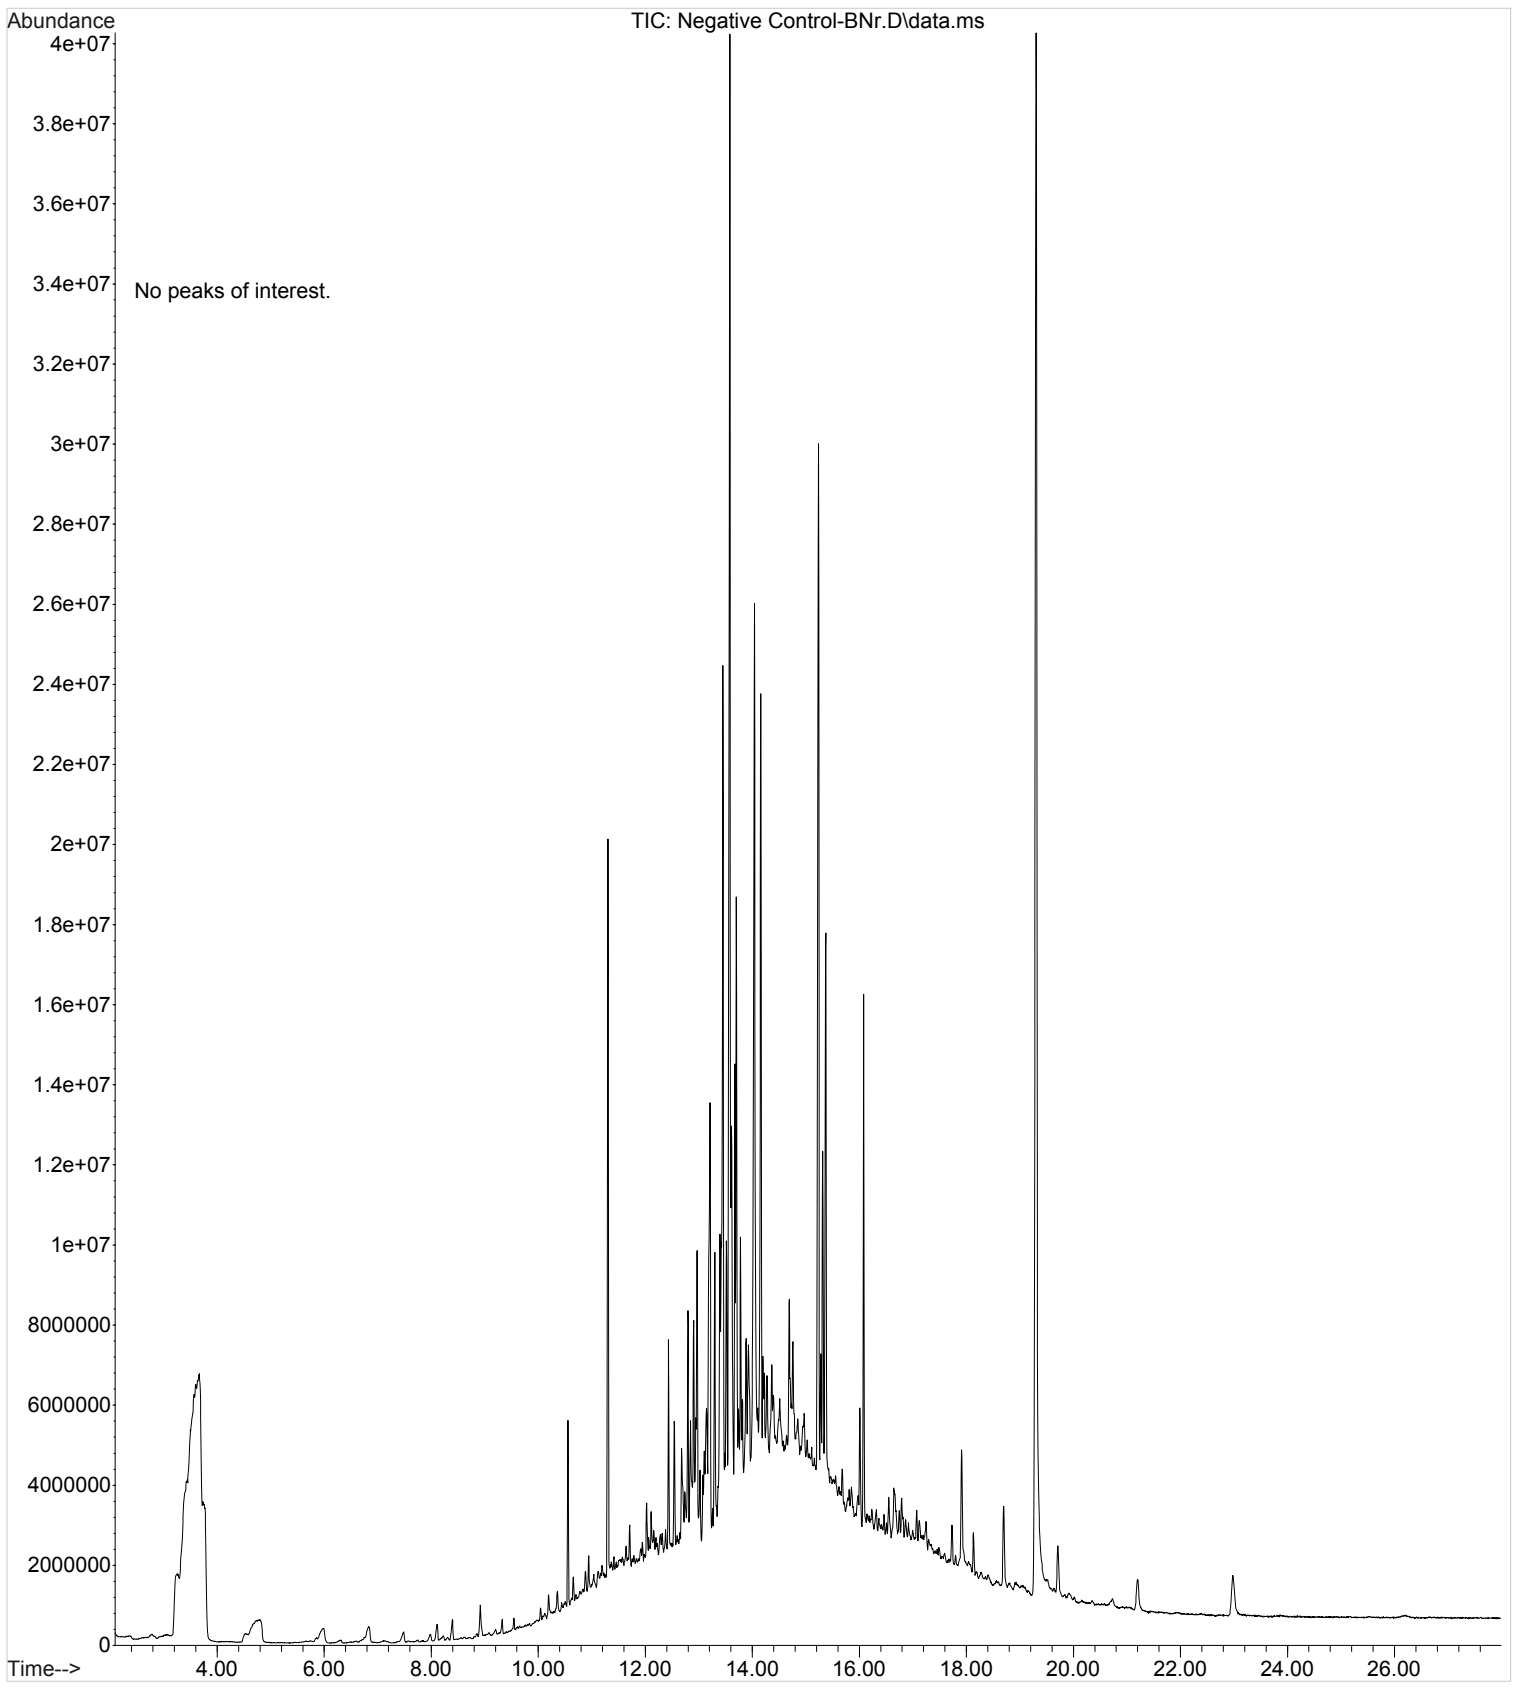



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\080516  
... \Negative Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 05 Aug 2016 17:39 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Negative Control - Utak Lot B1013  
Misc Info : Analytical Method 3.6.1

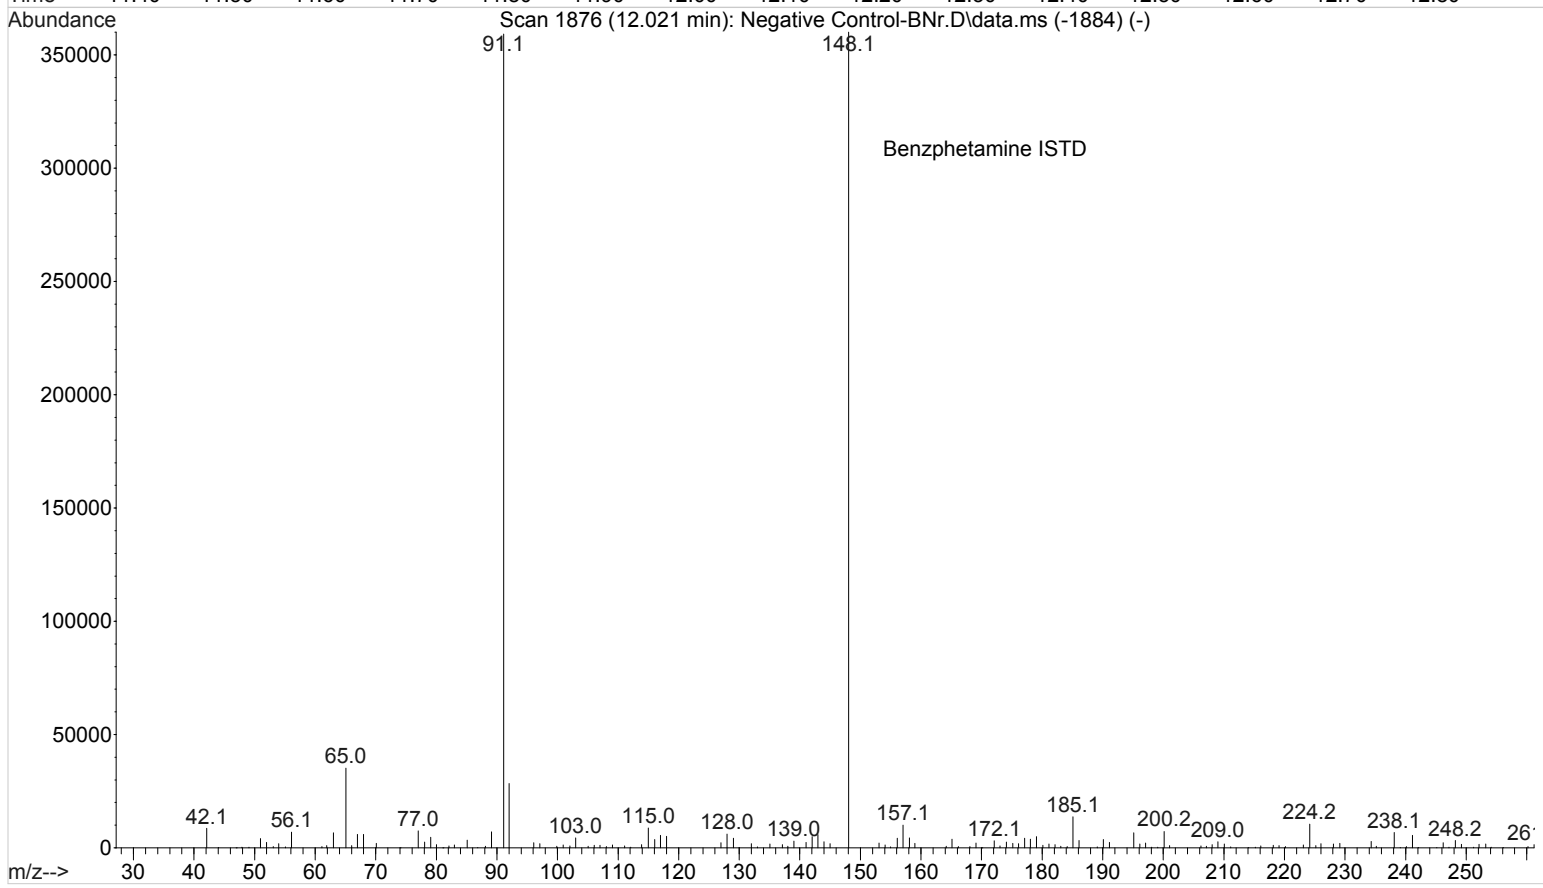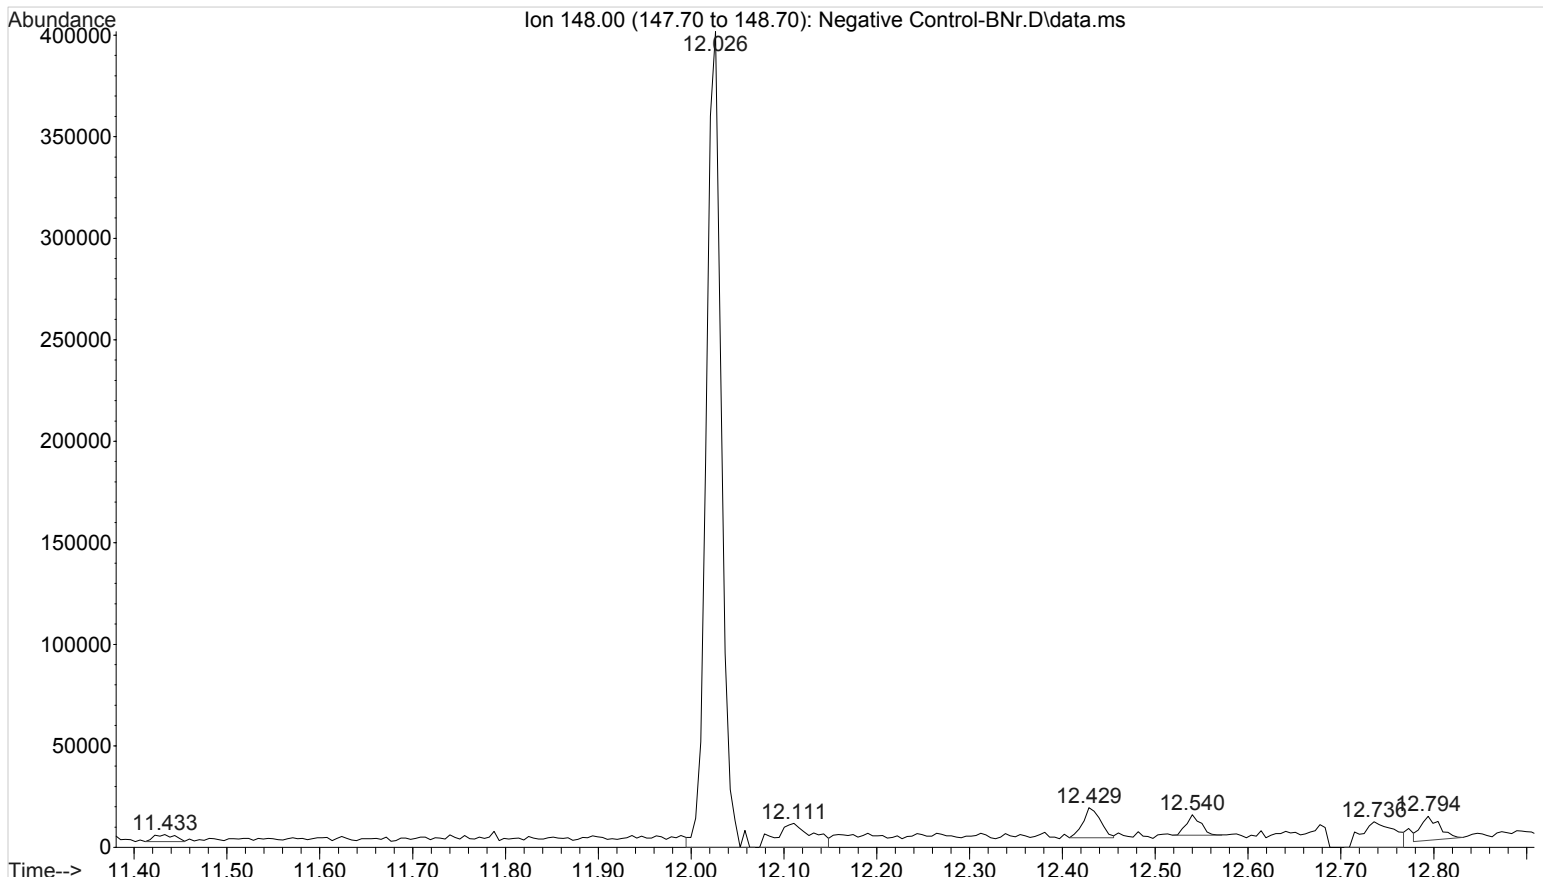



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\080516  
... \Negative Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 05 Aug 2016 17:39 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Negative Control - Utak Lot B1013  
Misc Info : Analytical Method 3.6.1

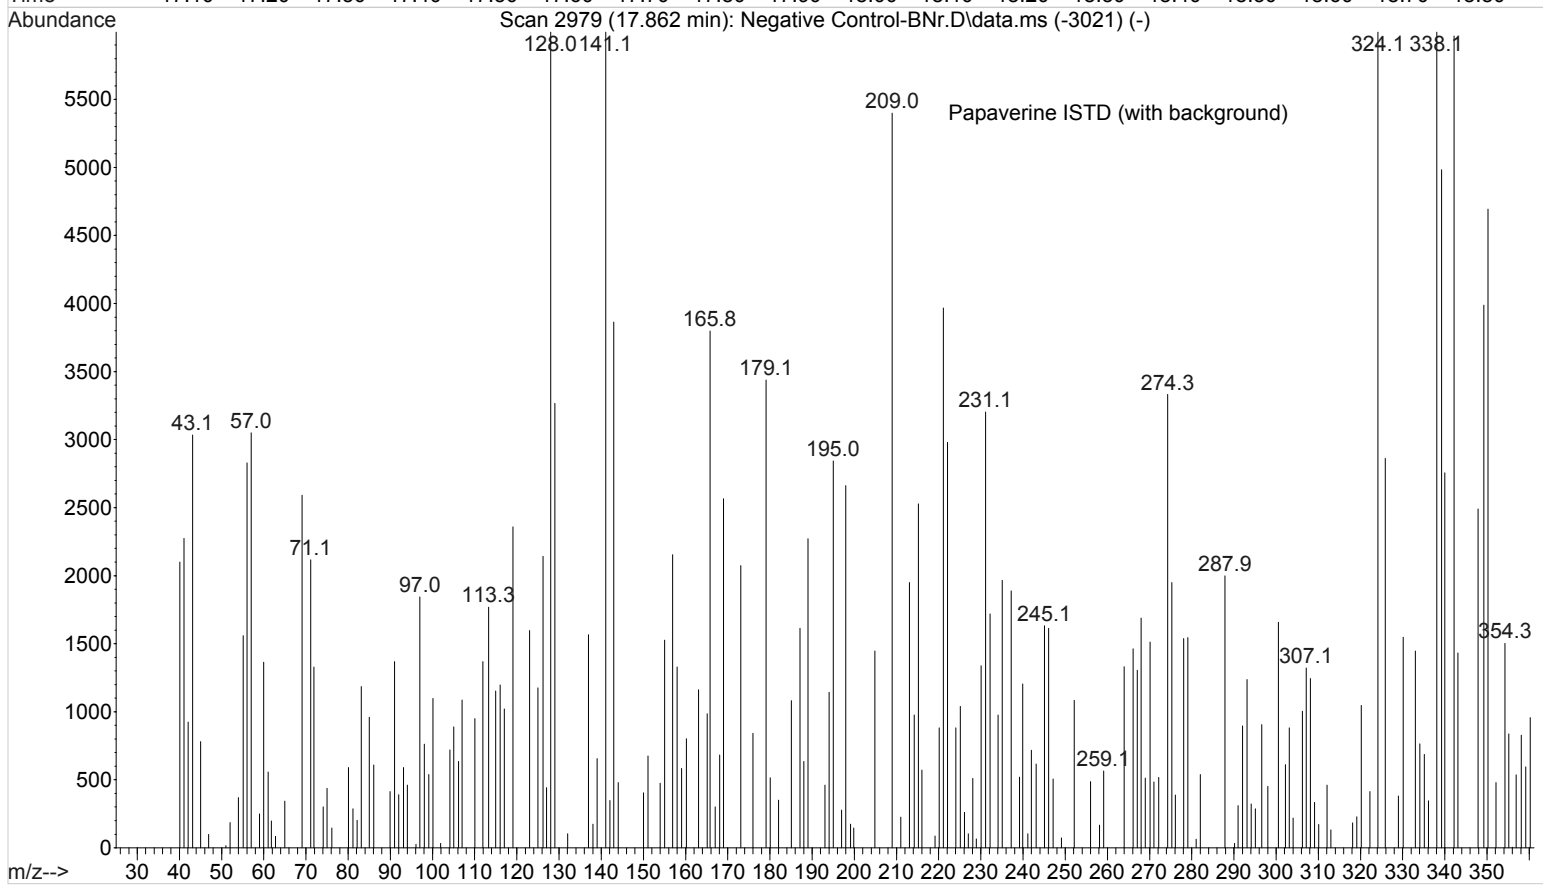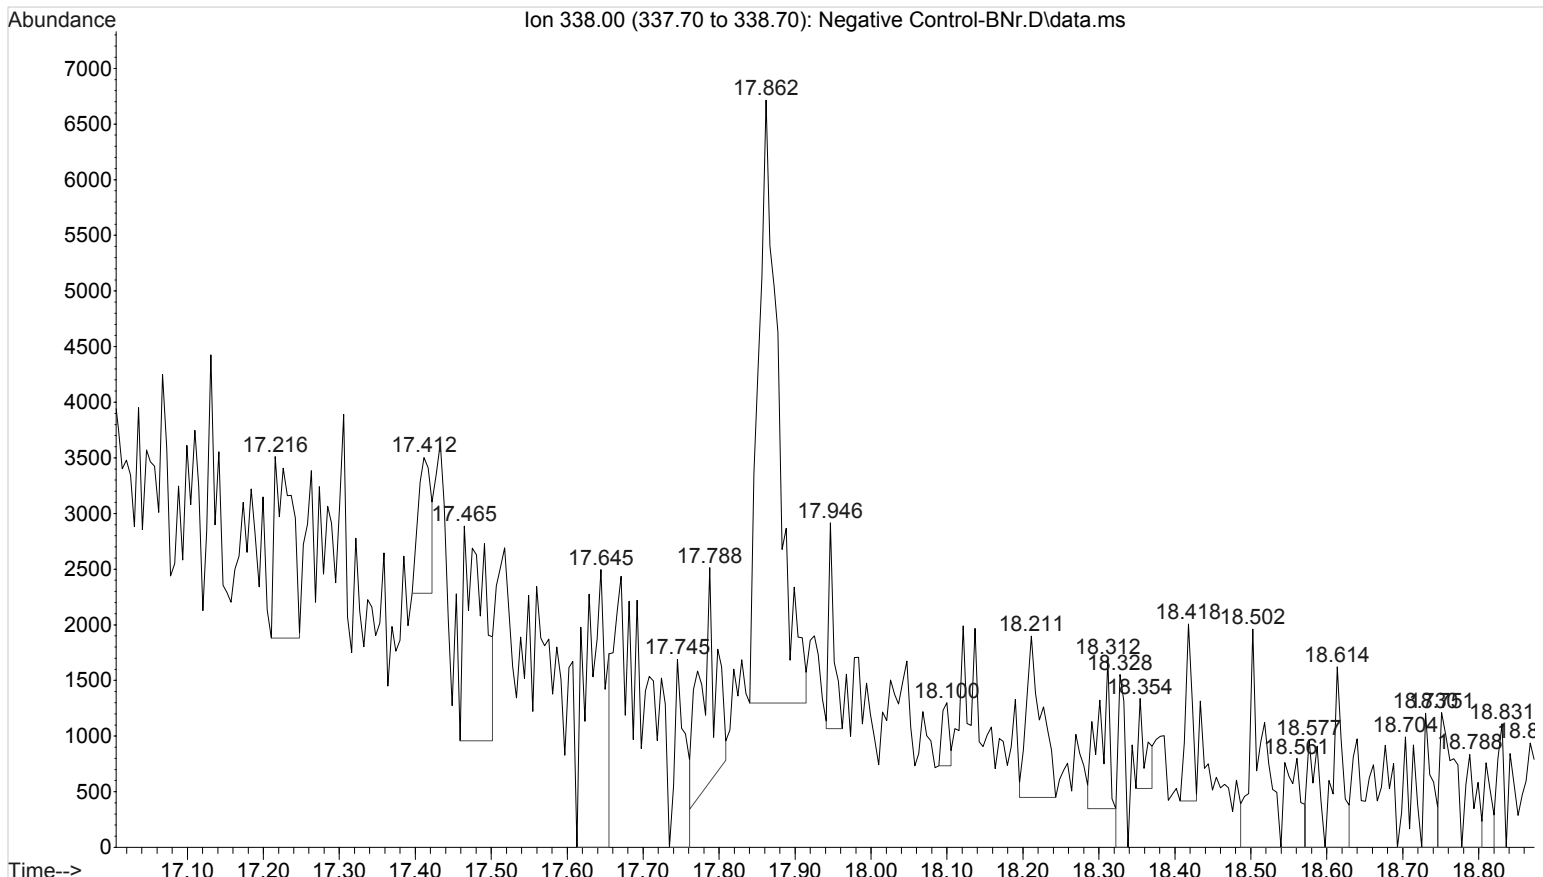



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\080516  
... \Spiked Positive Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 05 Aug 2016 18:13 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

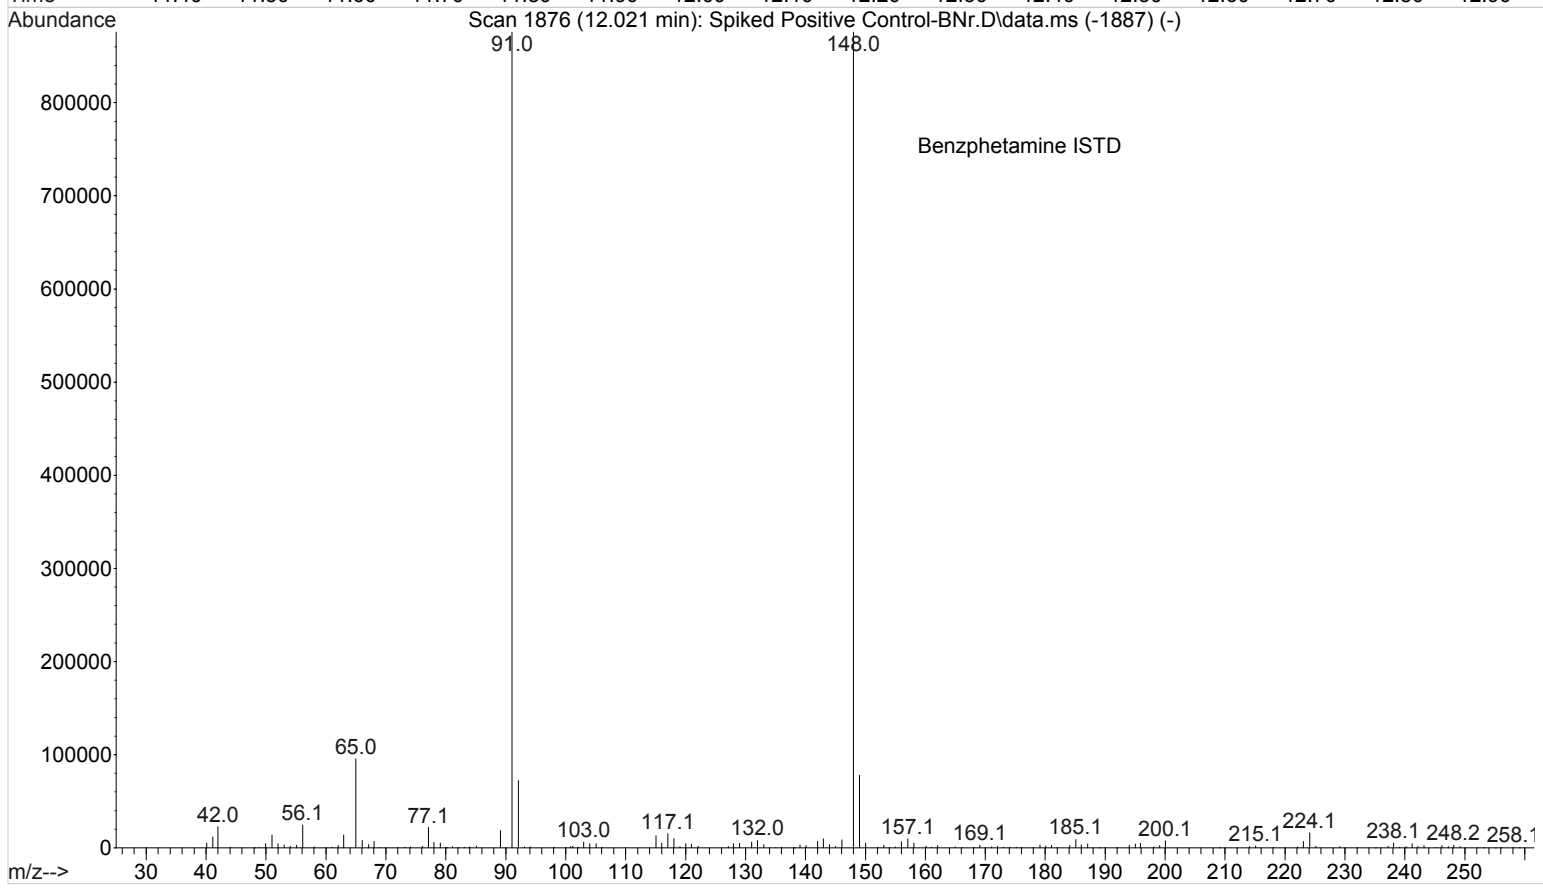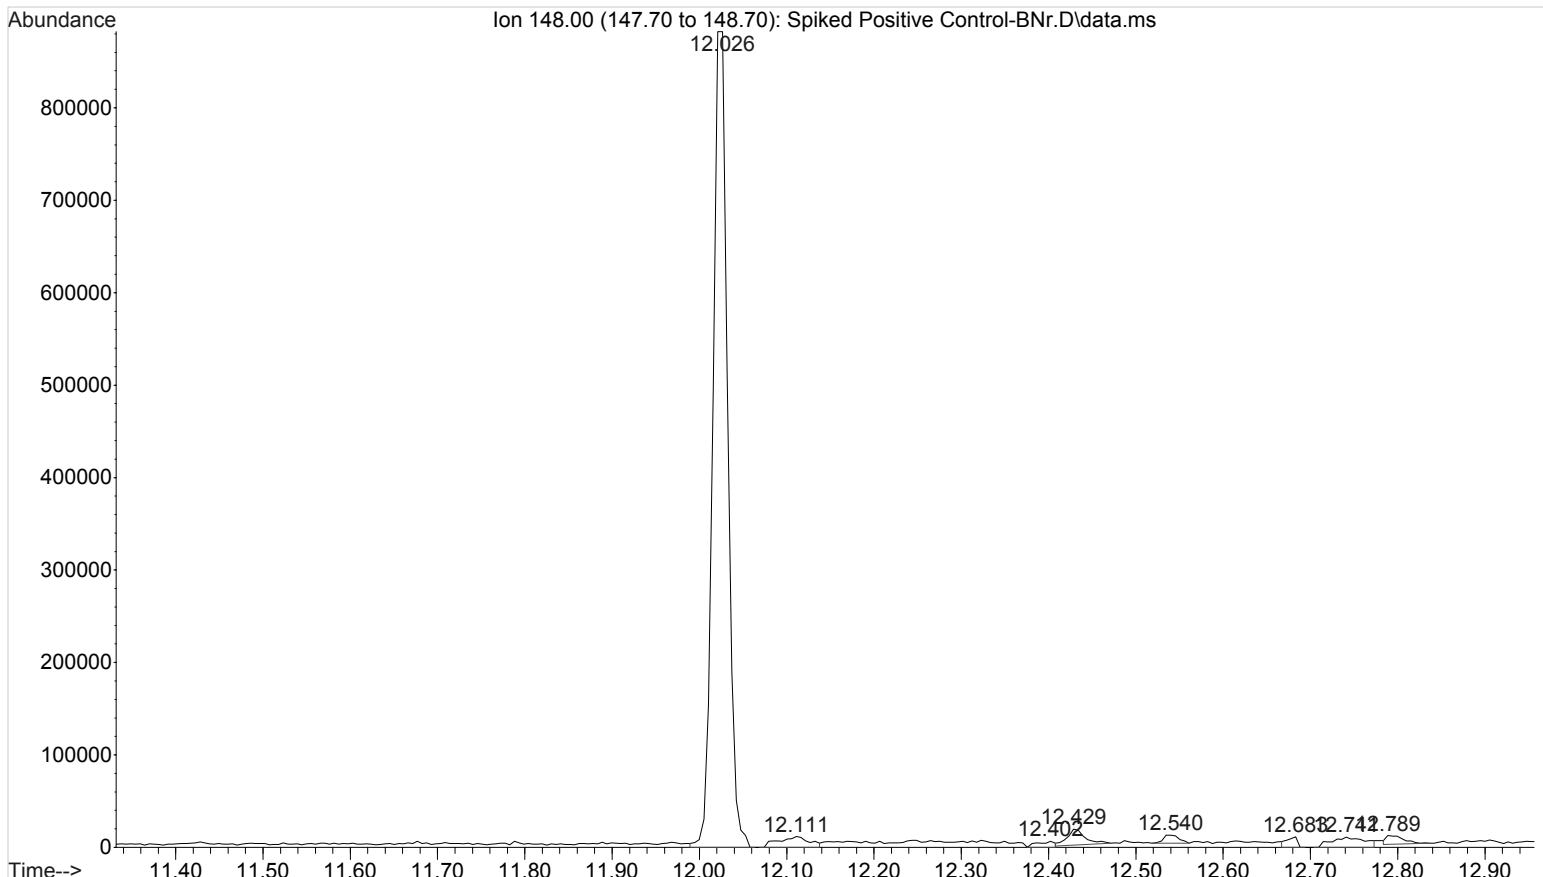



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\080516  
... \Spiked Positive Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 05 Aug 2016 18:13 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

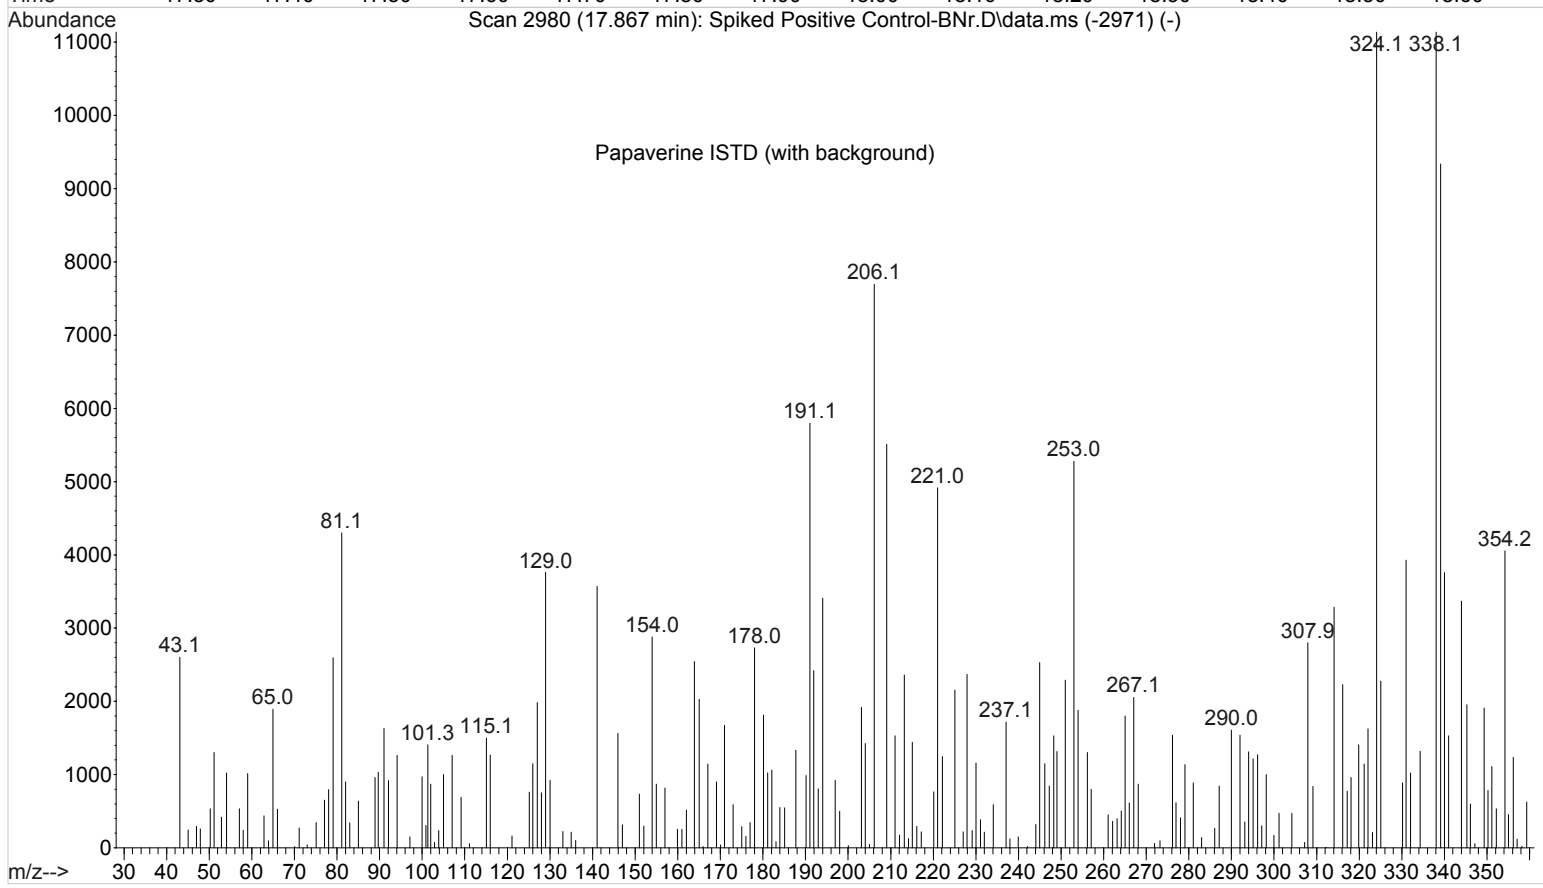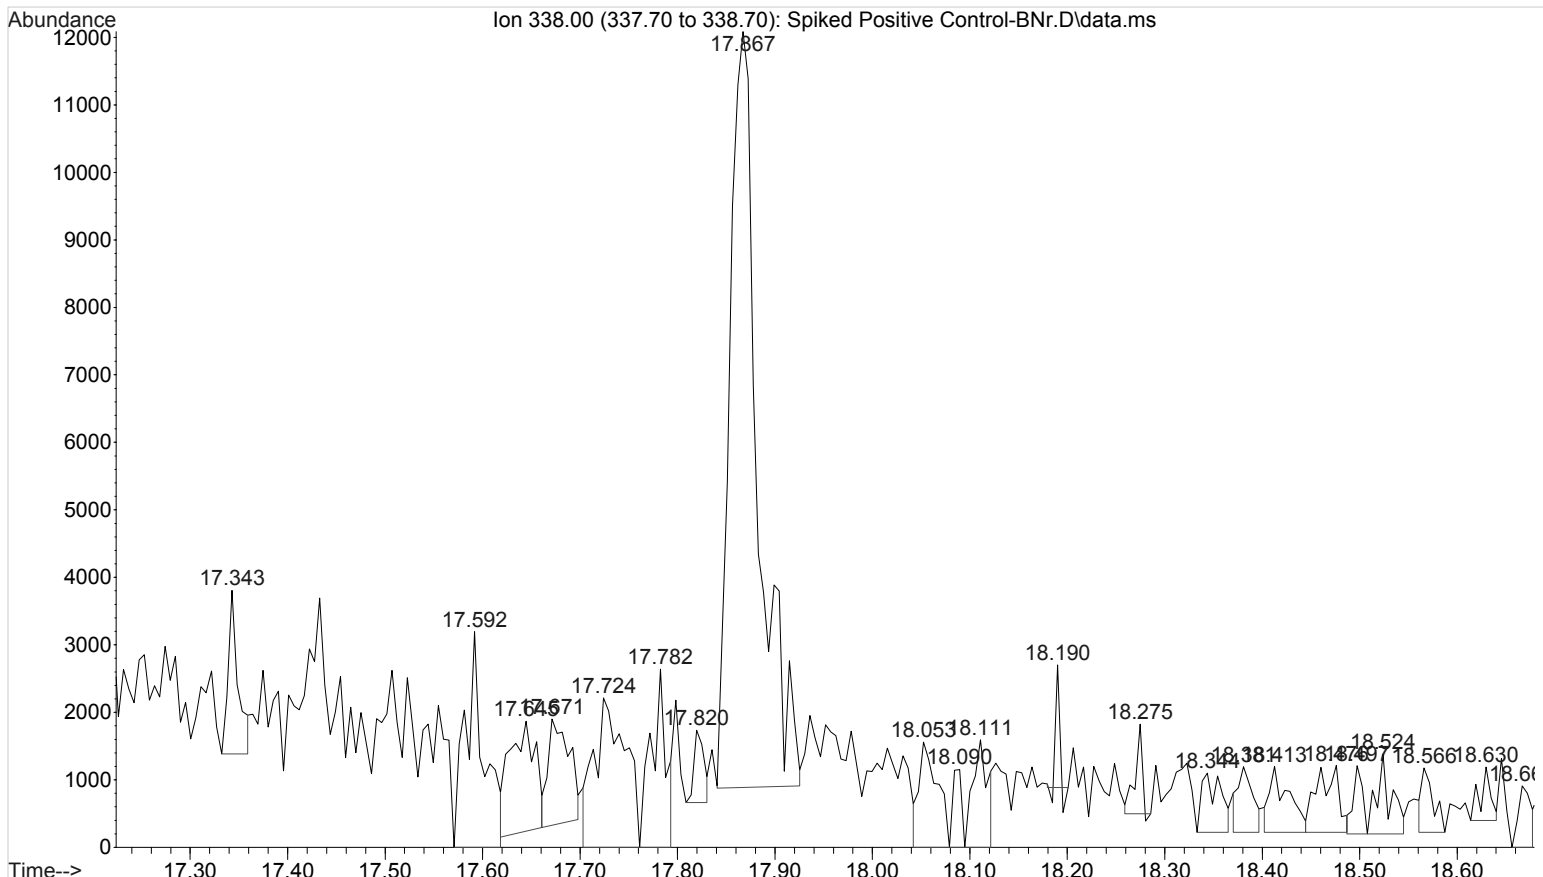

File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\080516  
... \Spiked Positive Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 05 Aug 2016 18:13 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

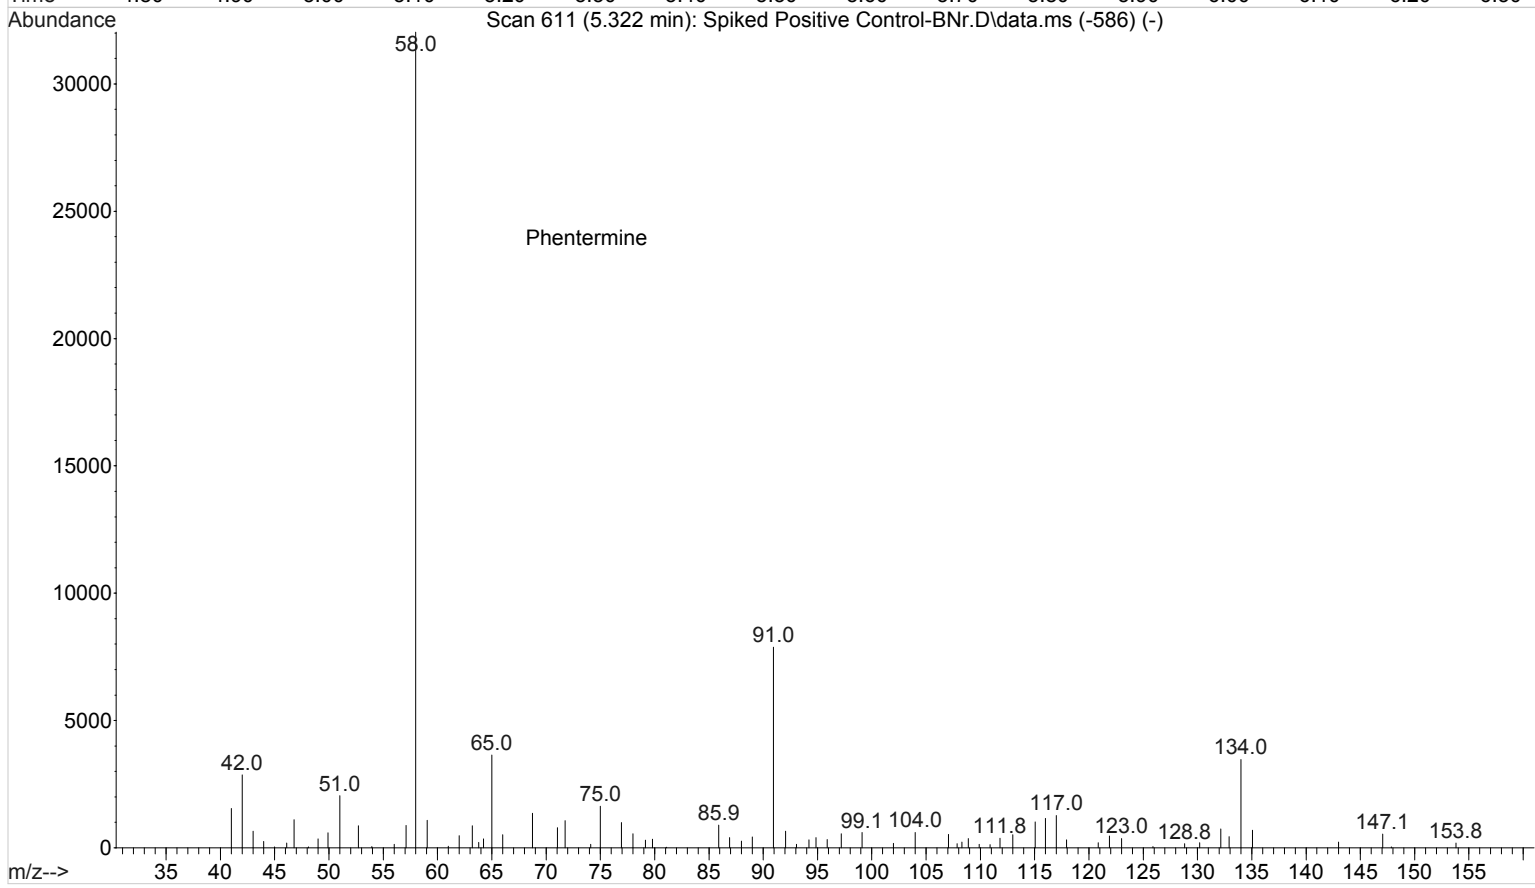
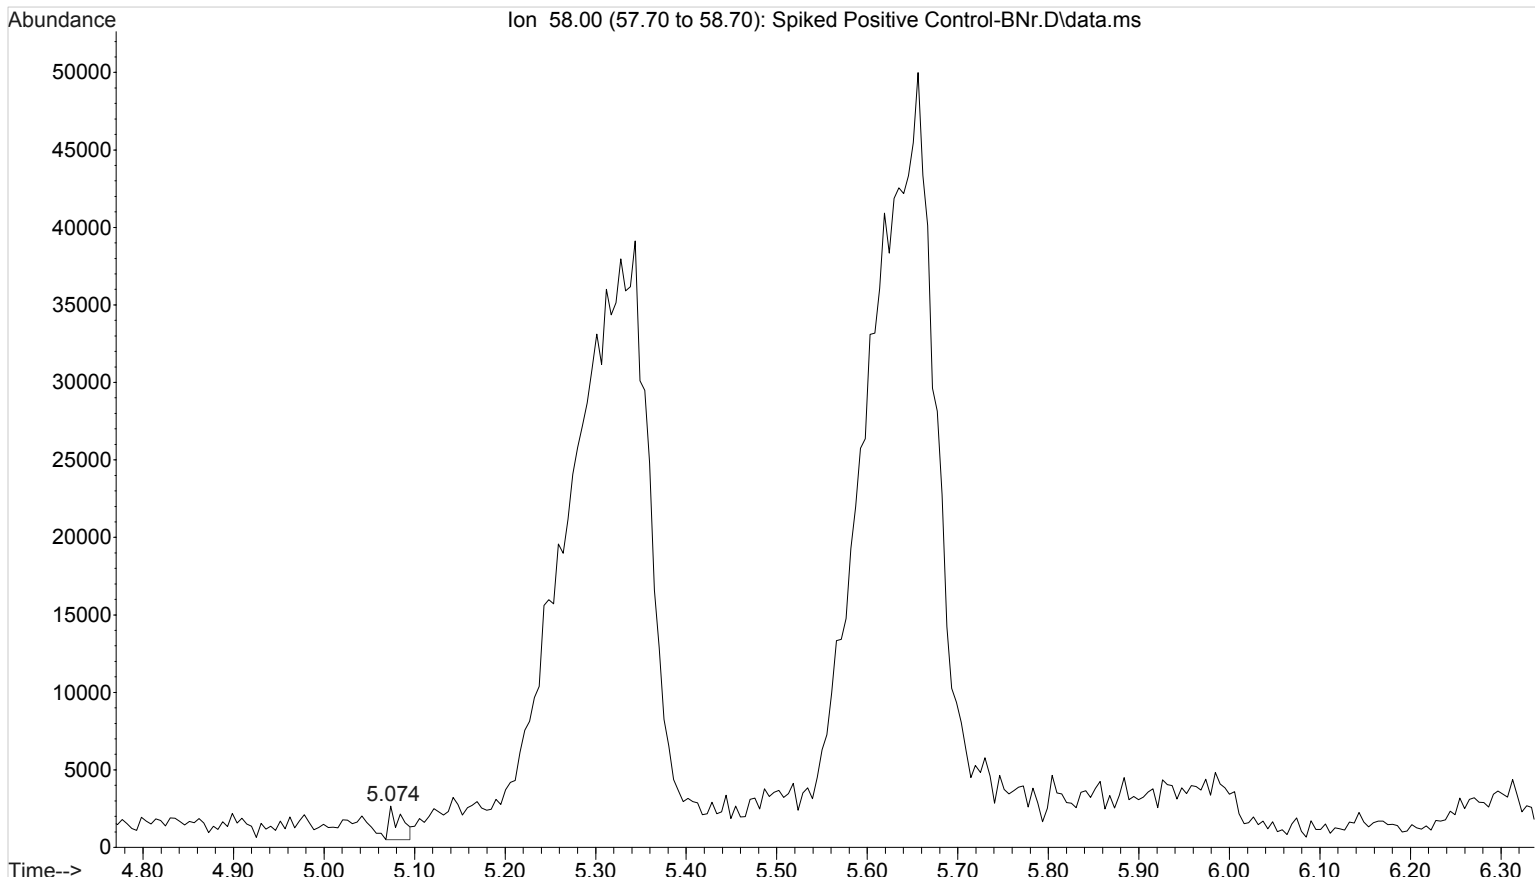


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\080516  
... \Spiked Positive Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 05 Aug 2016 18:13 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

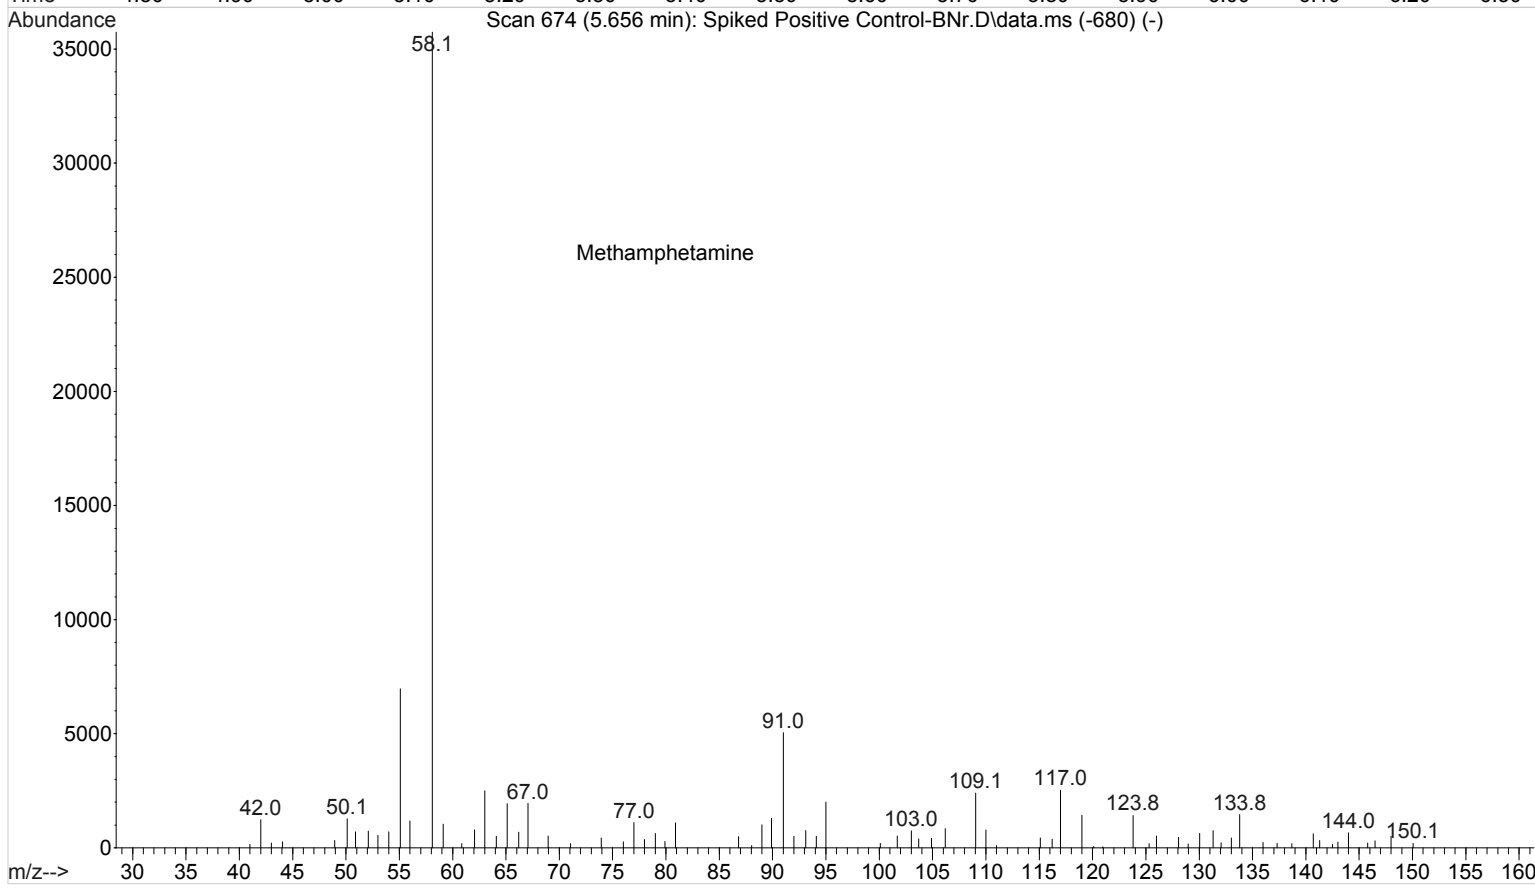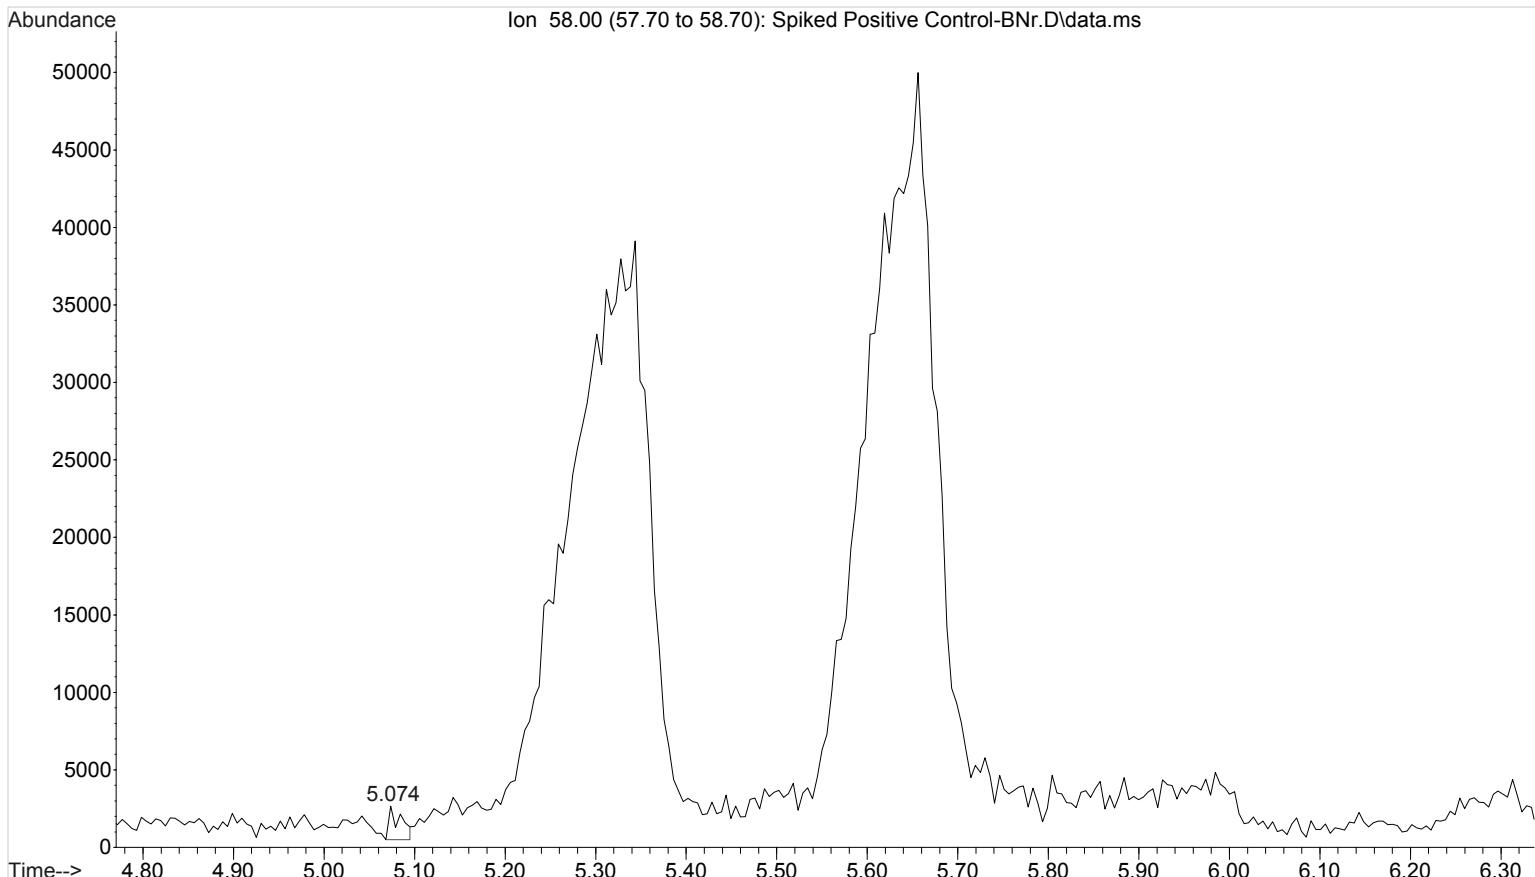

File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\080516  
... \Spiked Positive Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 05 Aug 2016 18:13 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215



CS

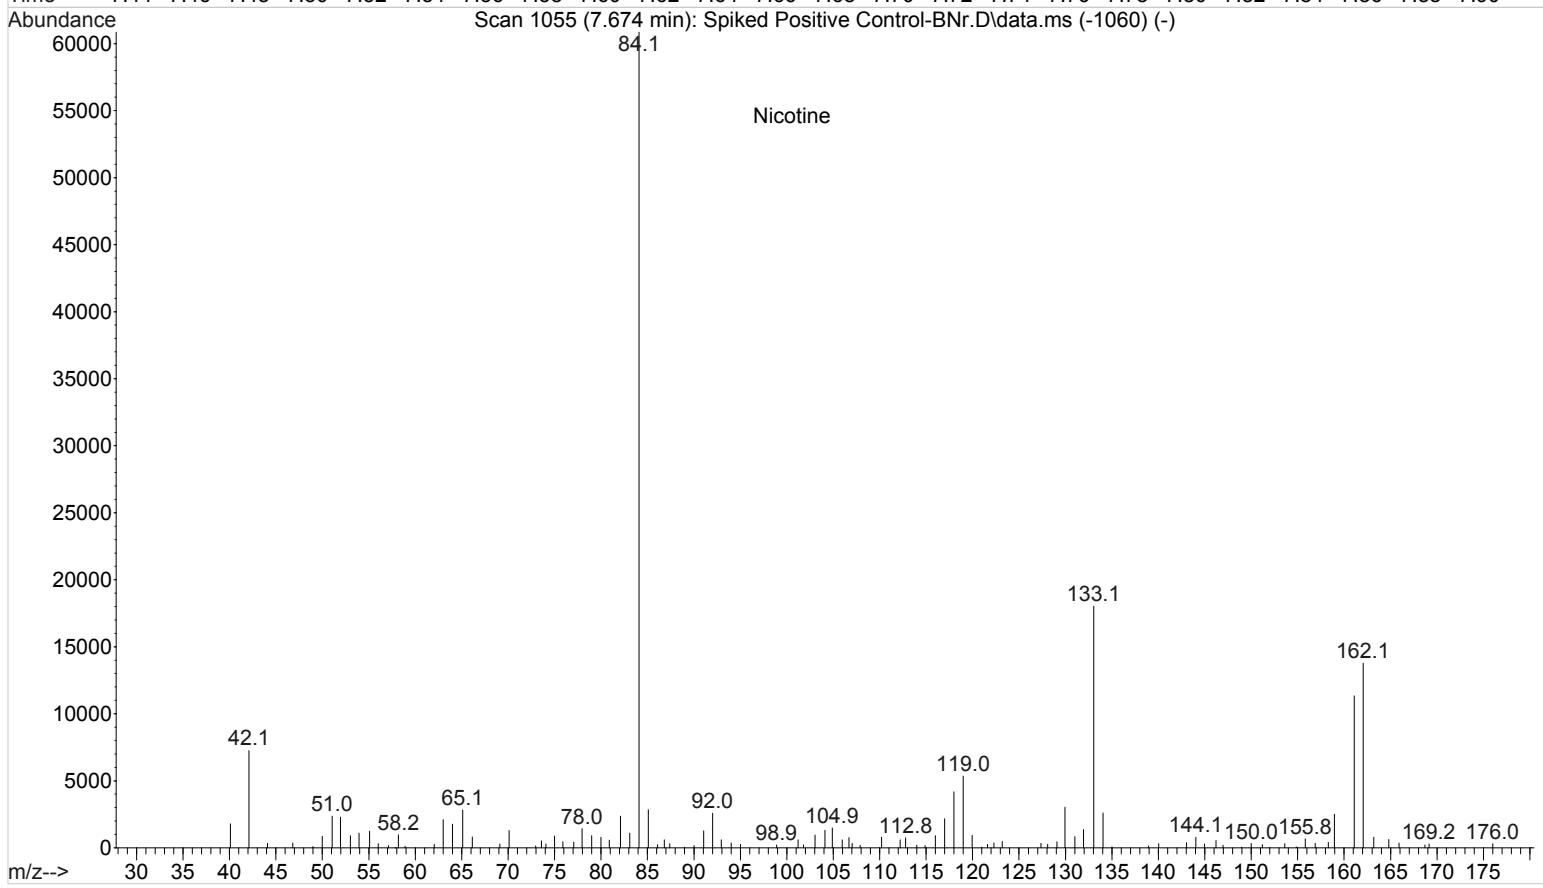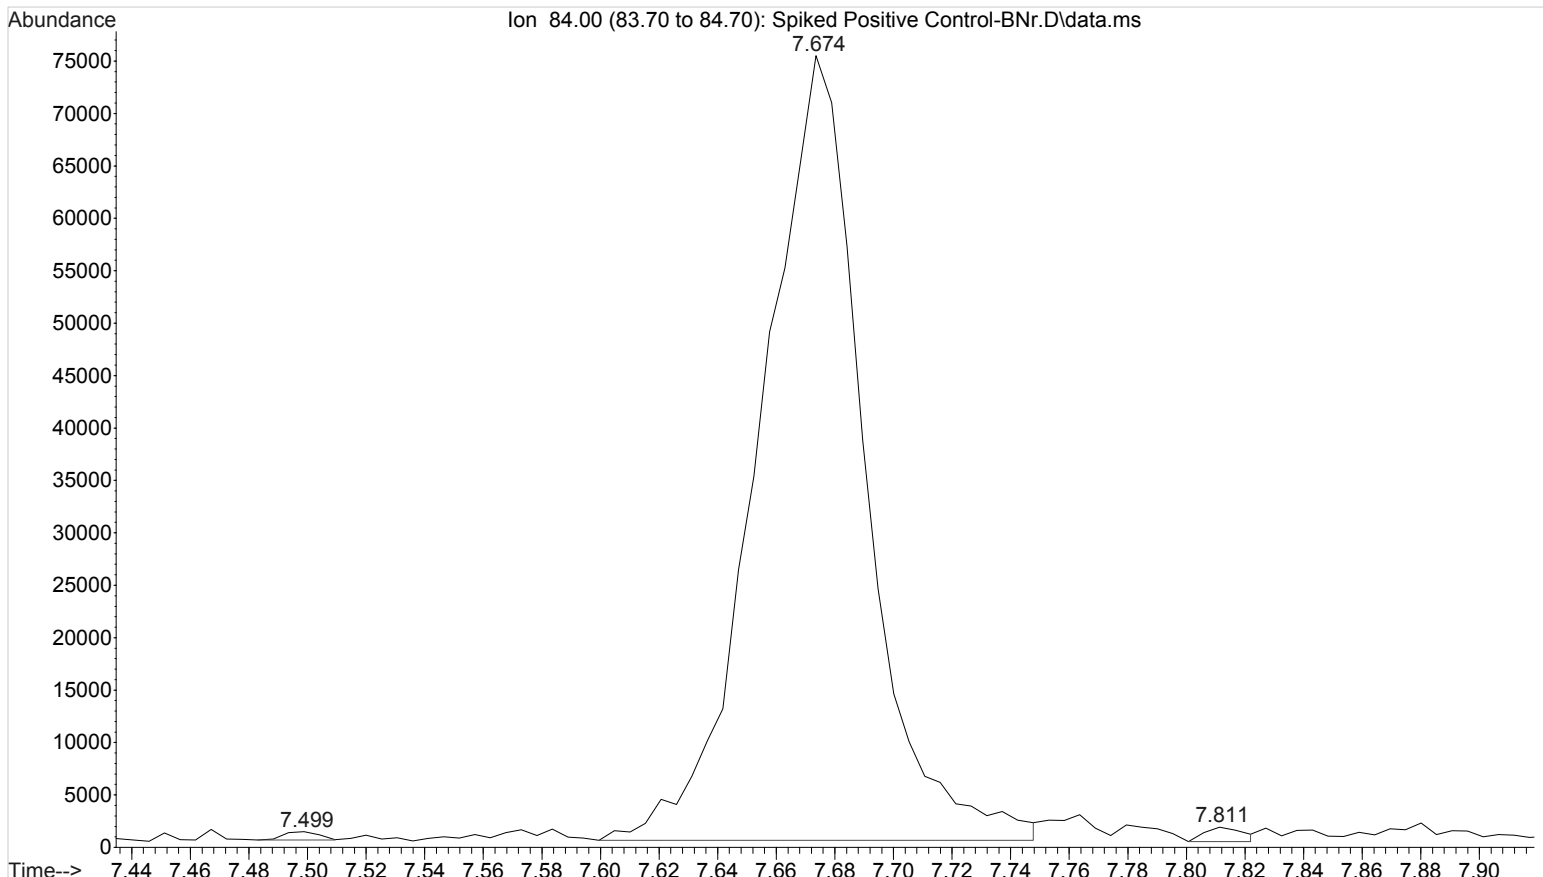





File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\080516  
... \Spiked Positive Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 05 Aug 2016 18:13 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215



6

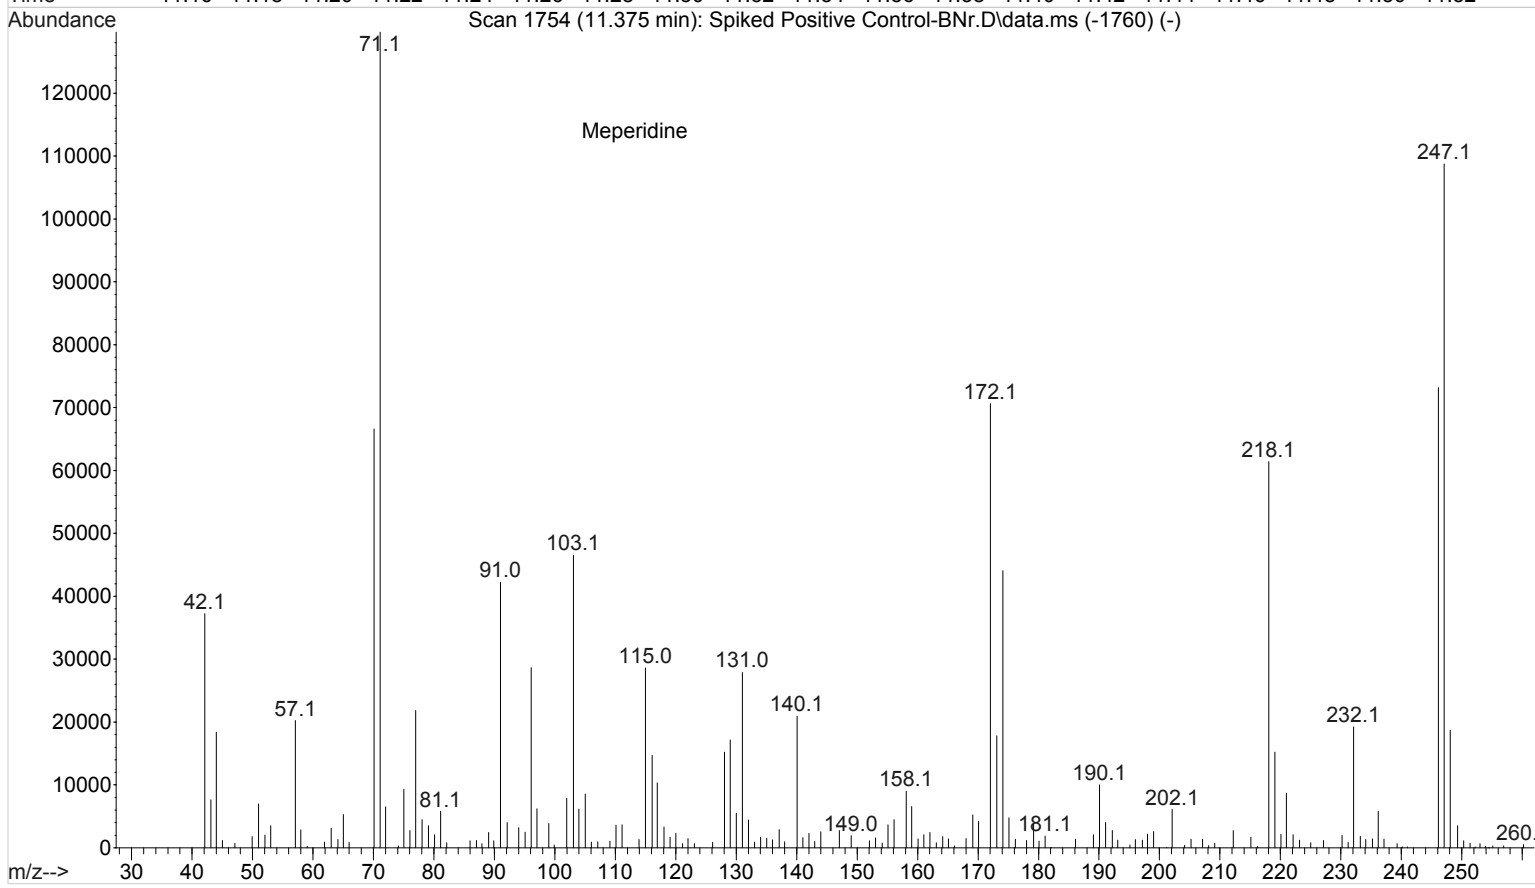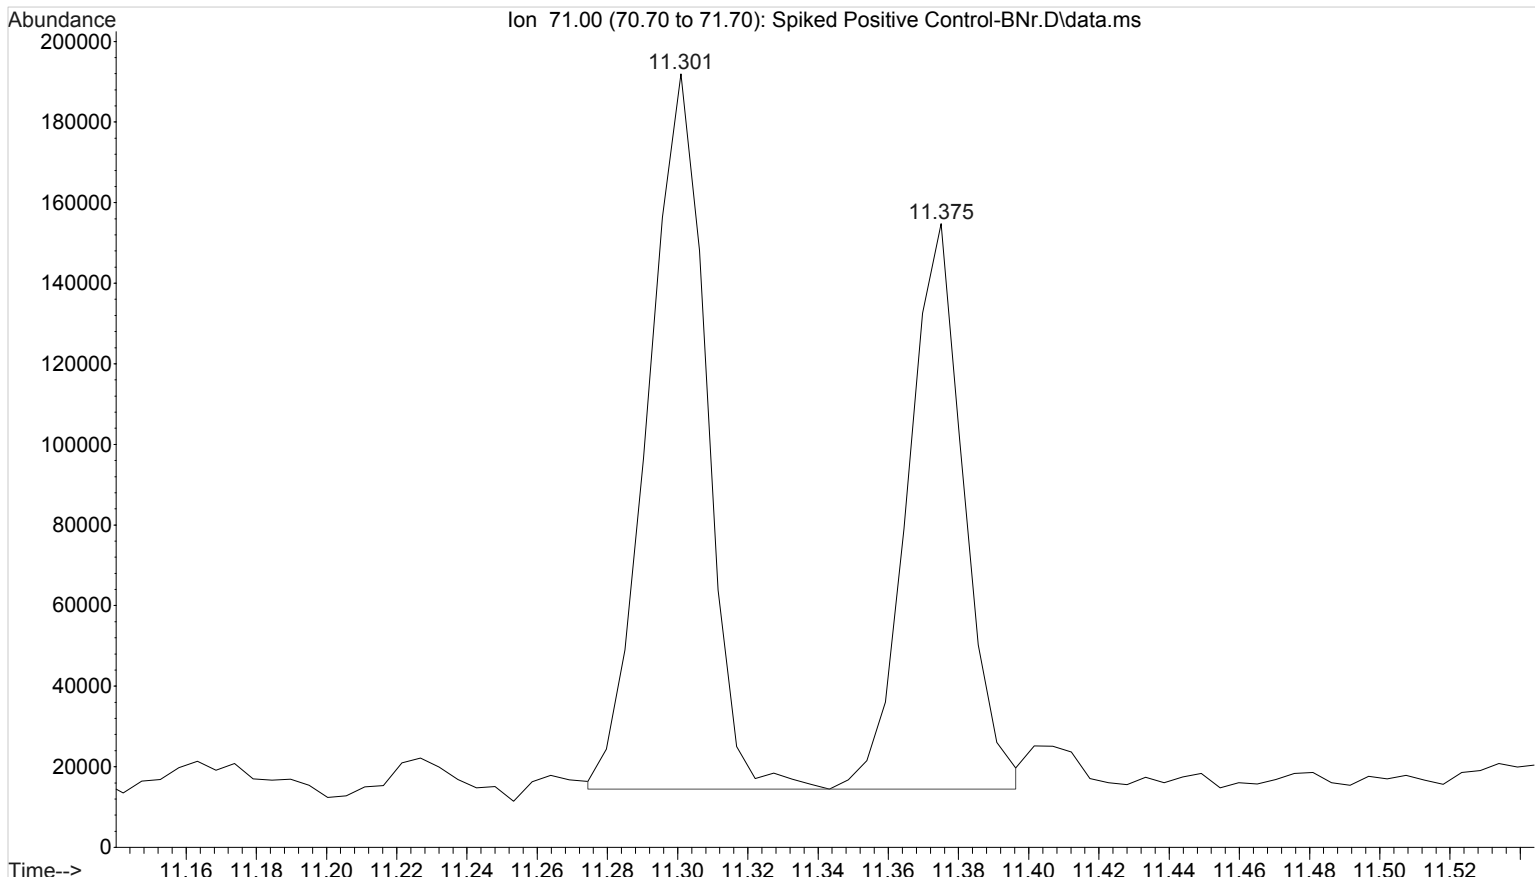



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\080516  
... \Spiked Positive Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 05 Aug 2016 18:13 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

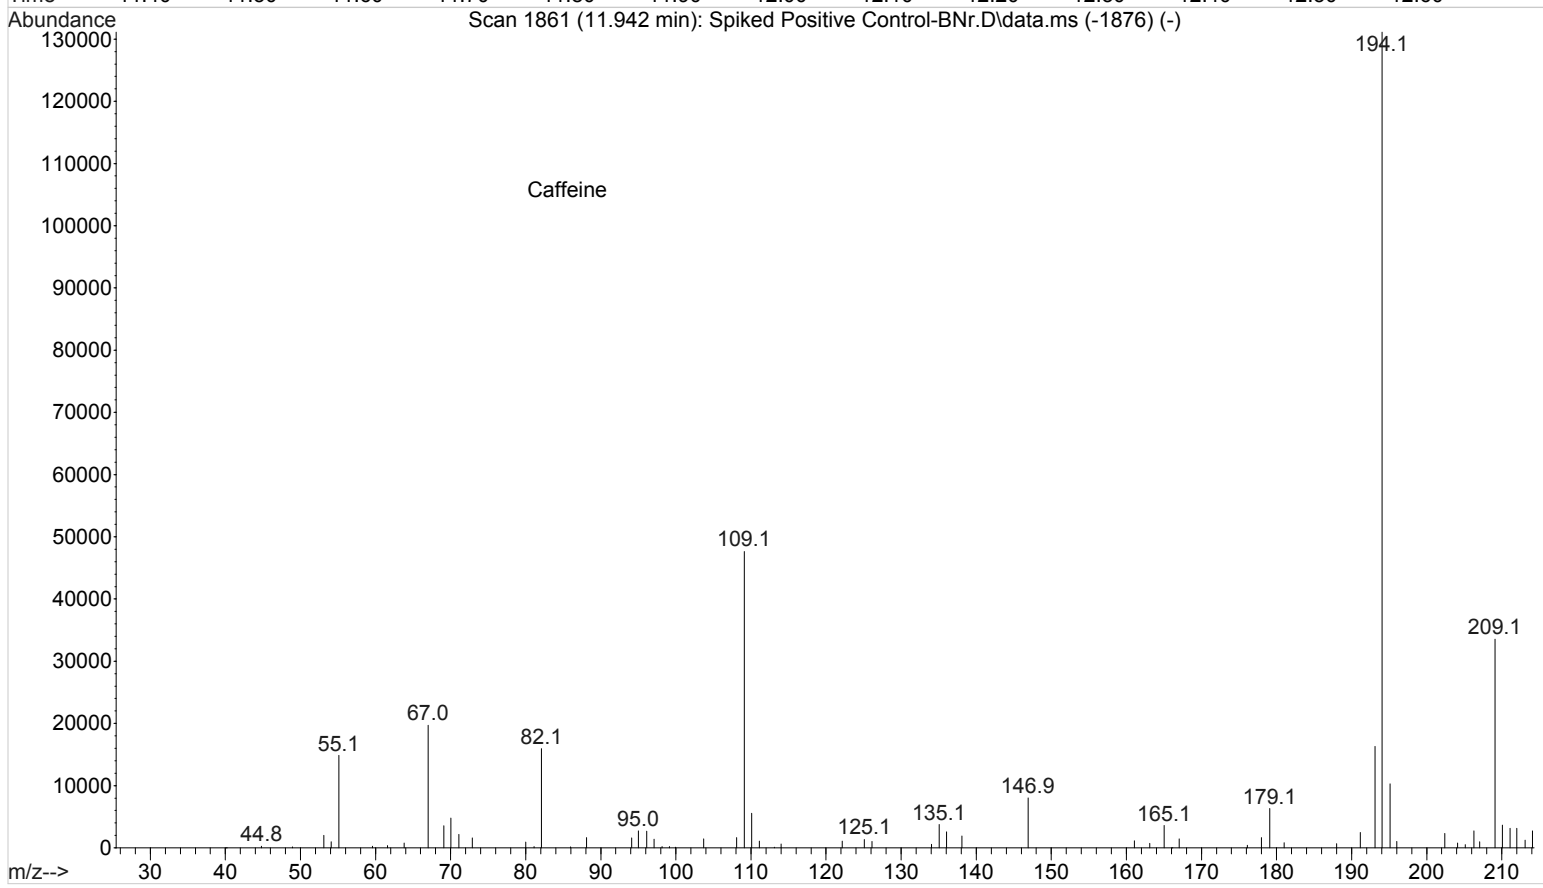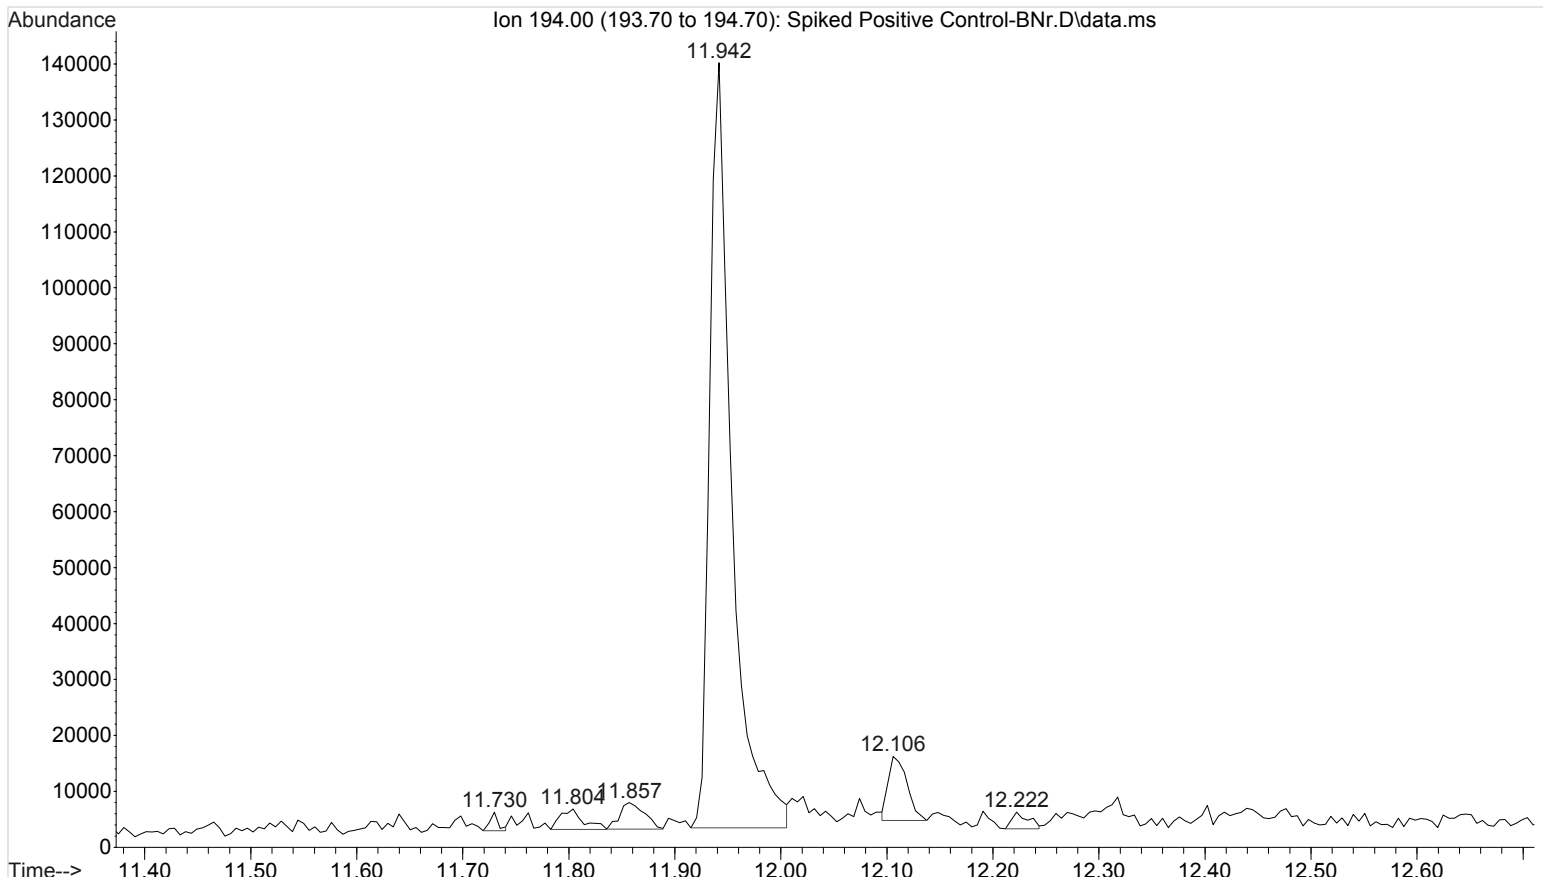



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\080516  
... \Spiked Positive Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 05 Aug 2016 18:13 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

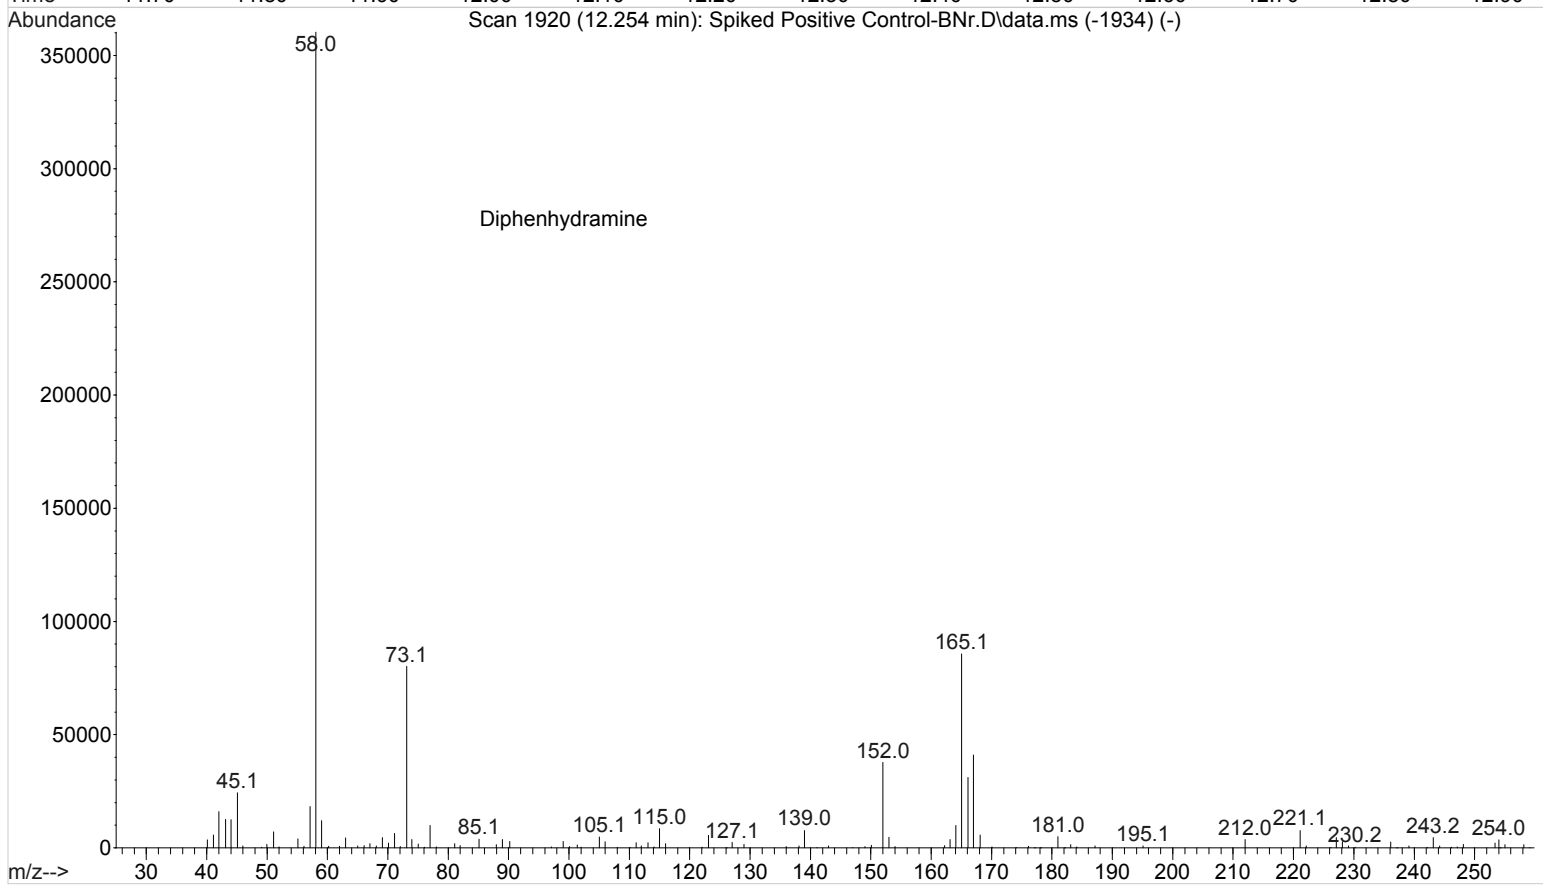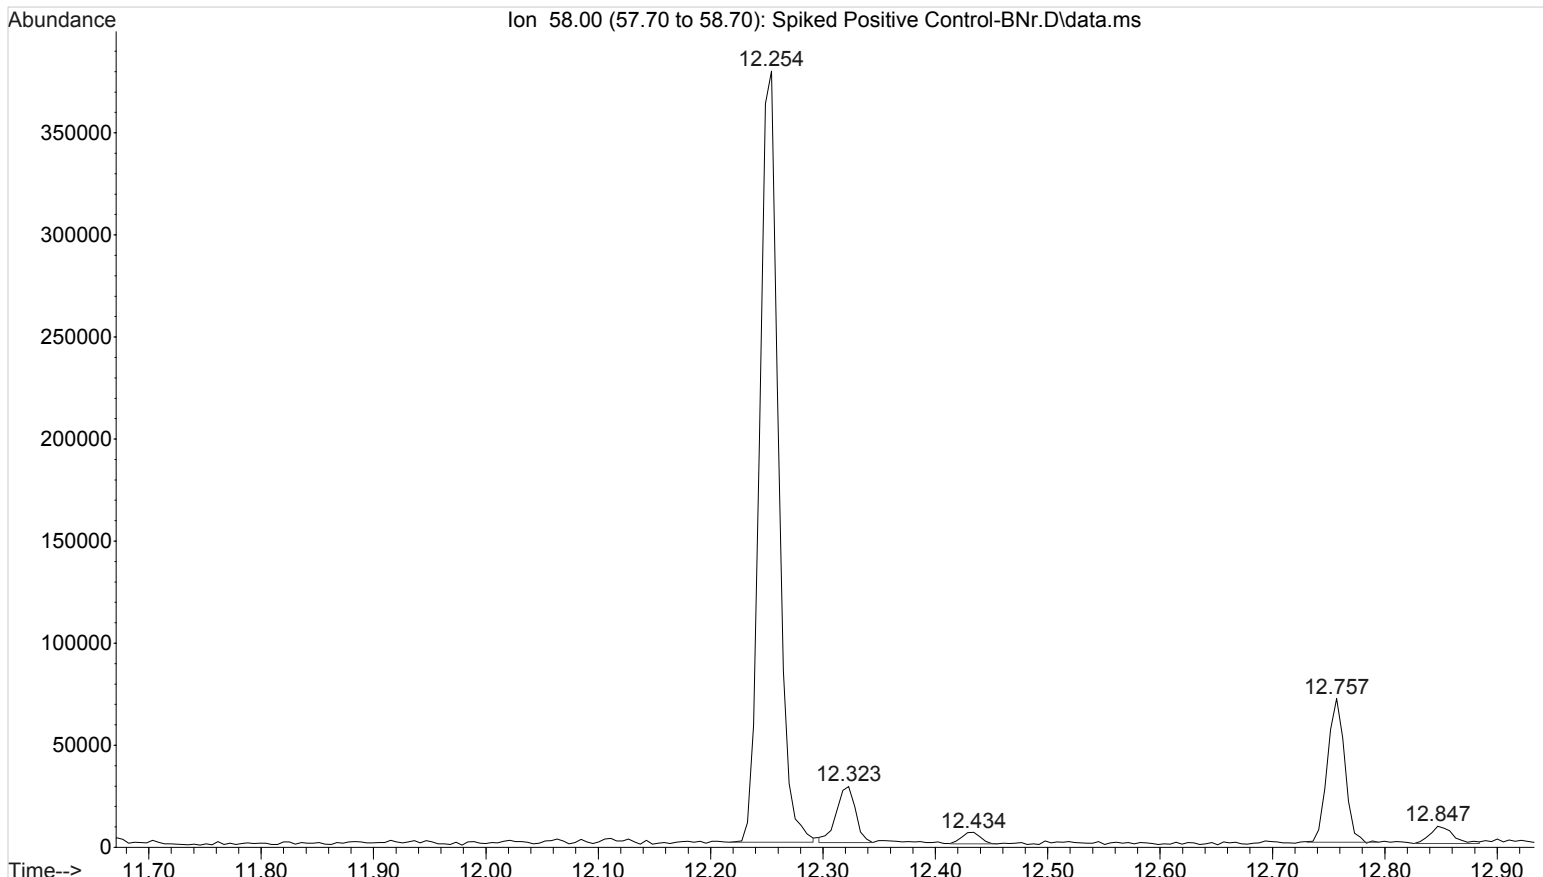



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\080516  
... \Spiked Positive Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 05 Aug 2016 18:13 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

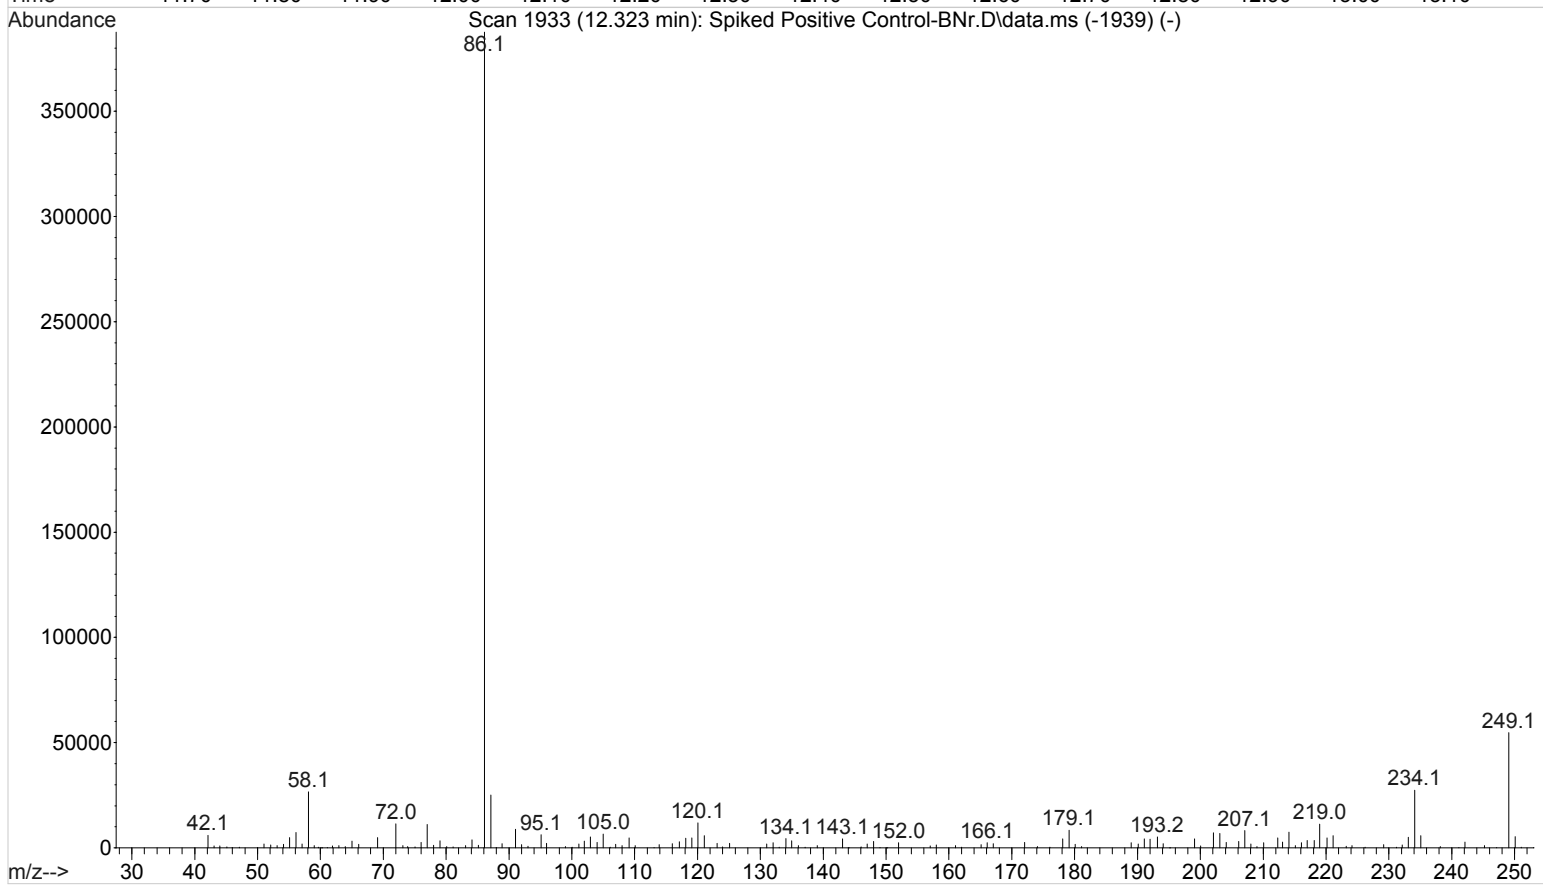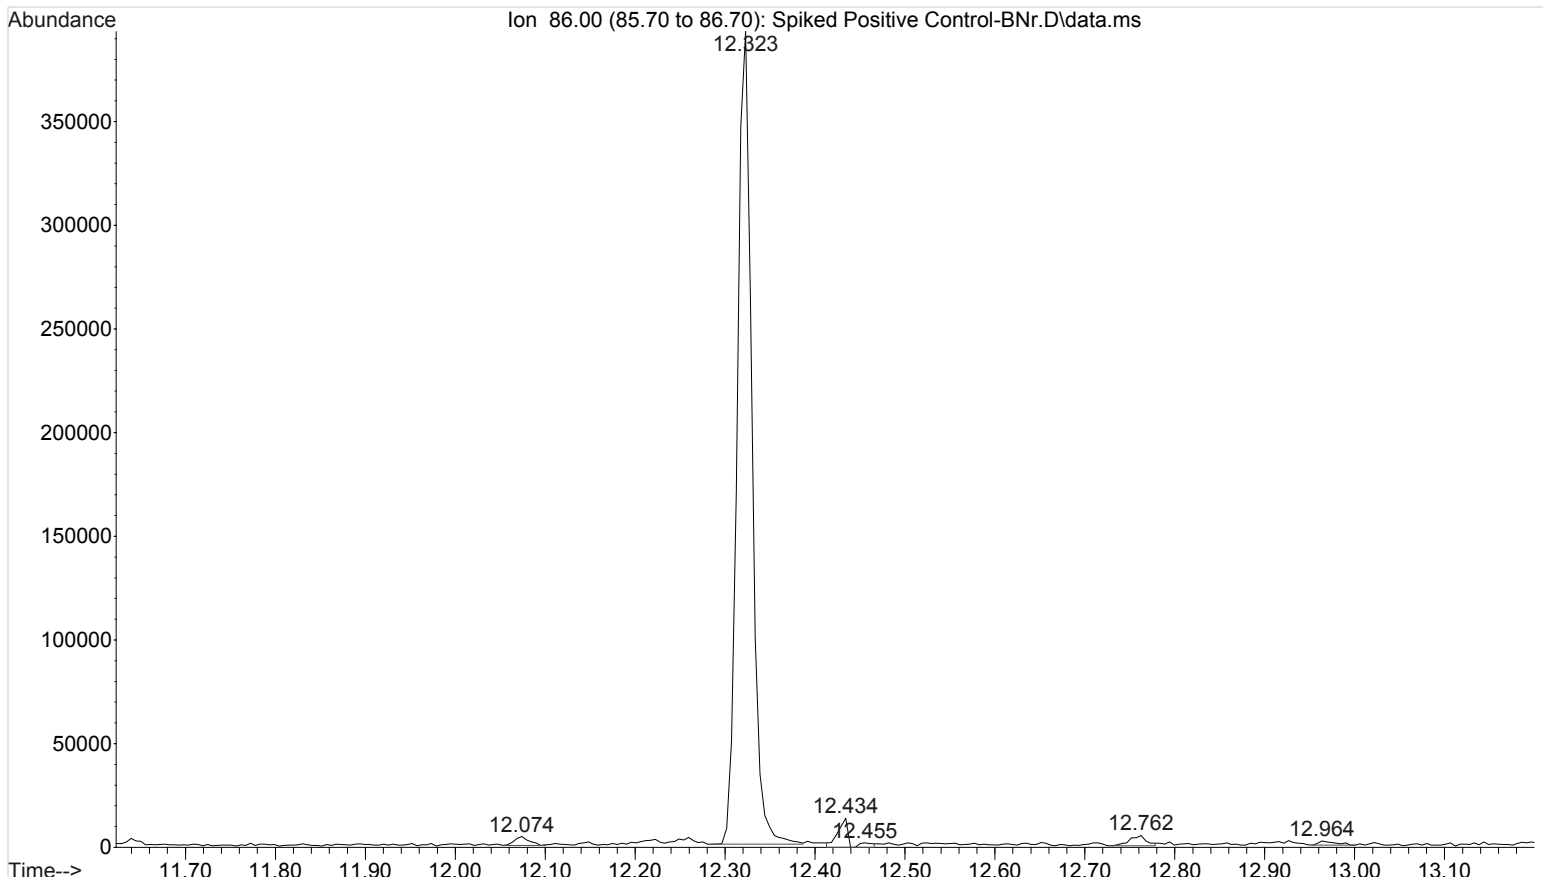

File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\080516  
... \Spiked Positive Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 05 Aug 2016 18:13 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

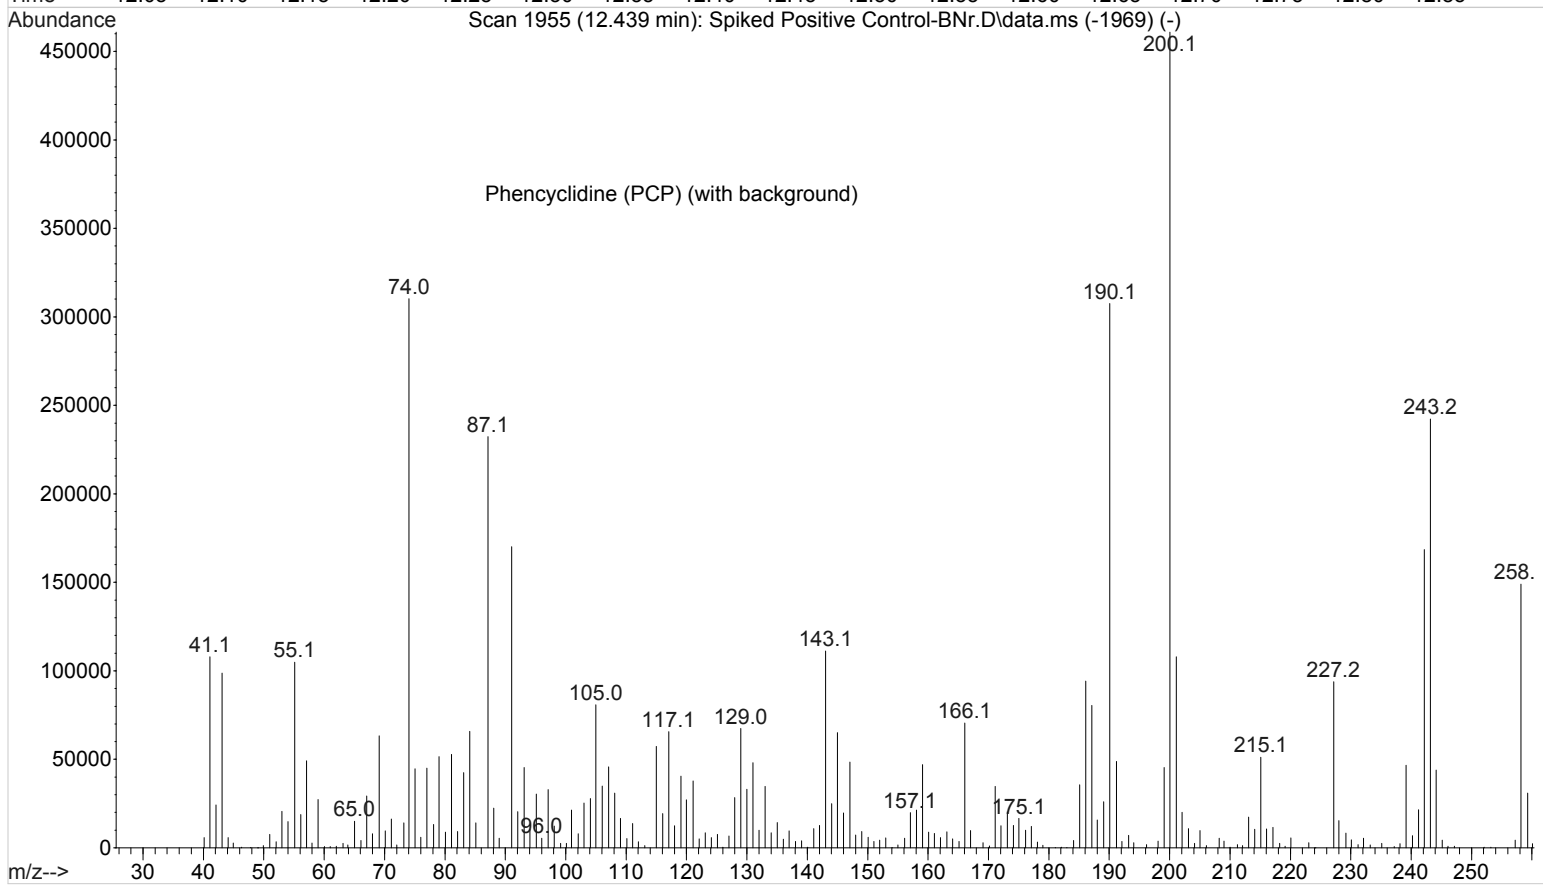
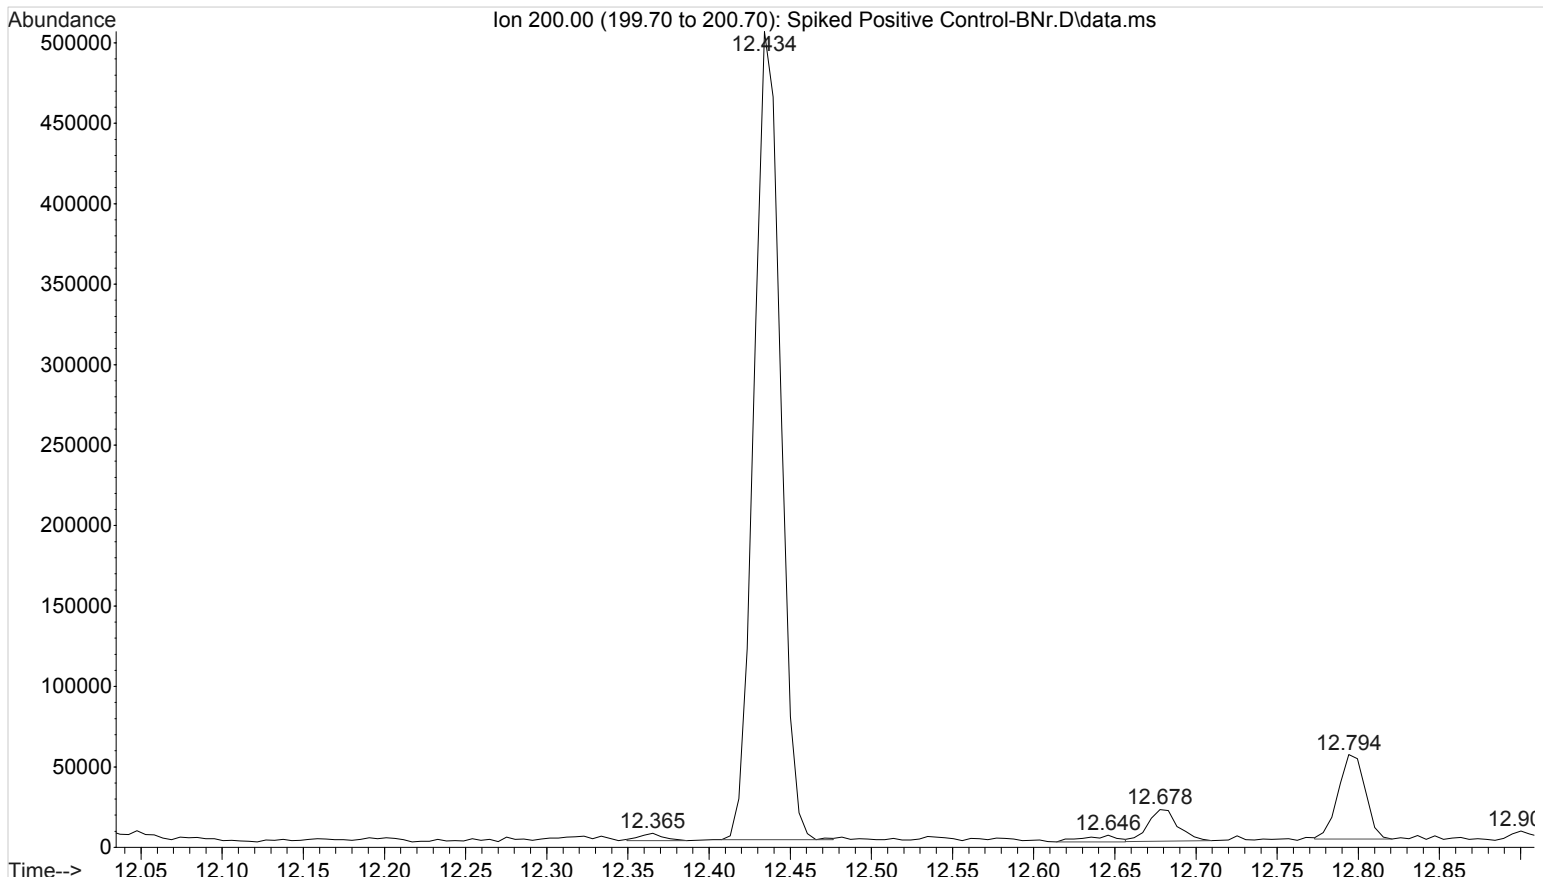


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\080516  
... \Spiked Positive Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 05 Aug 2016 18:13 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

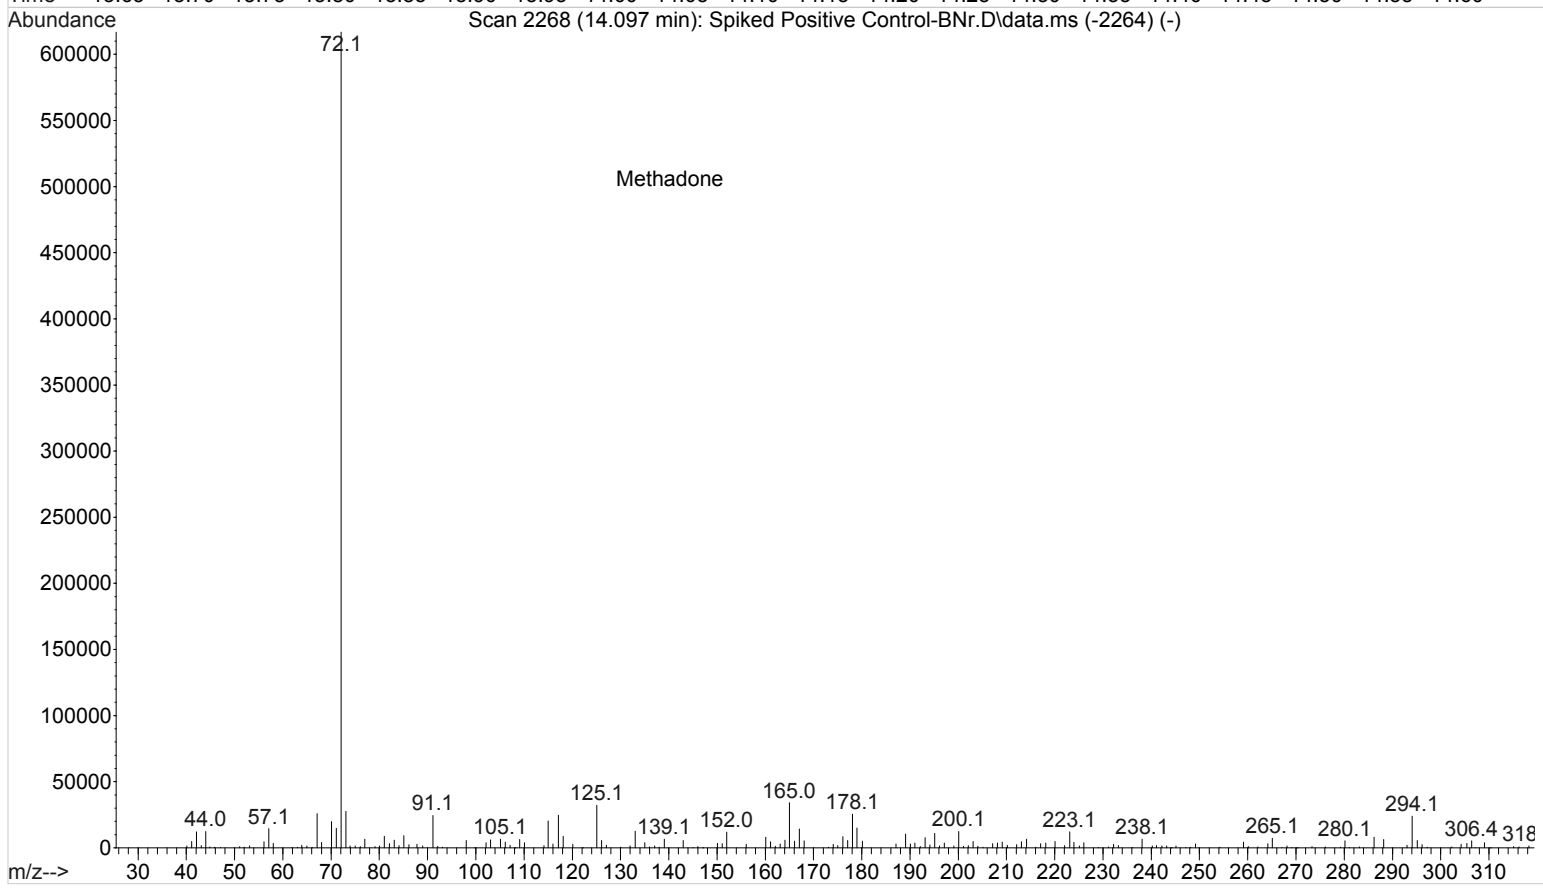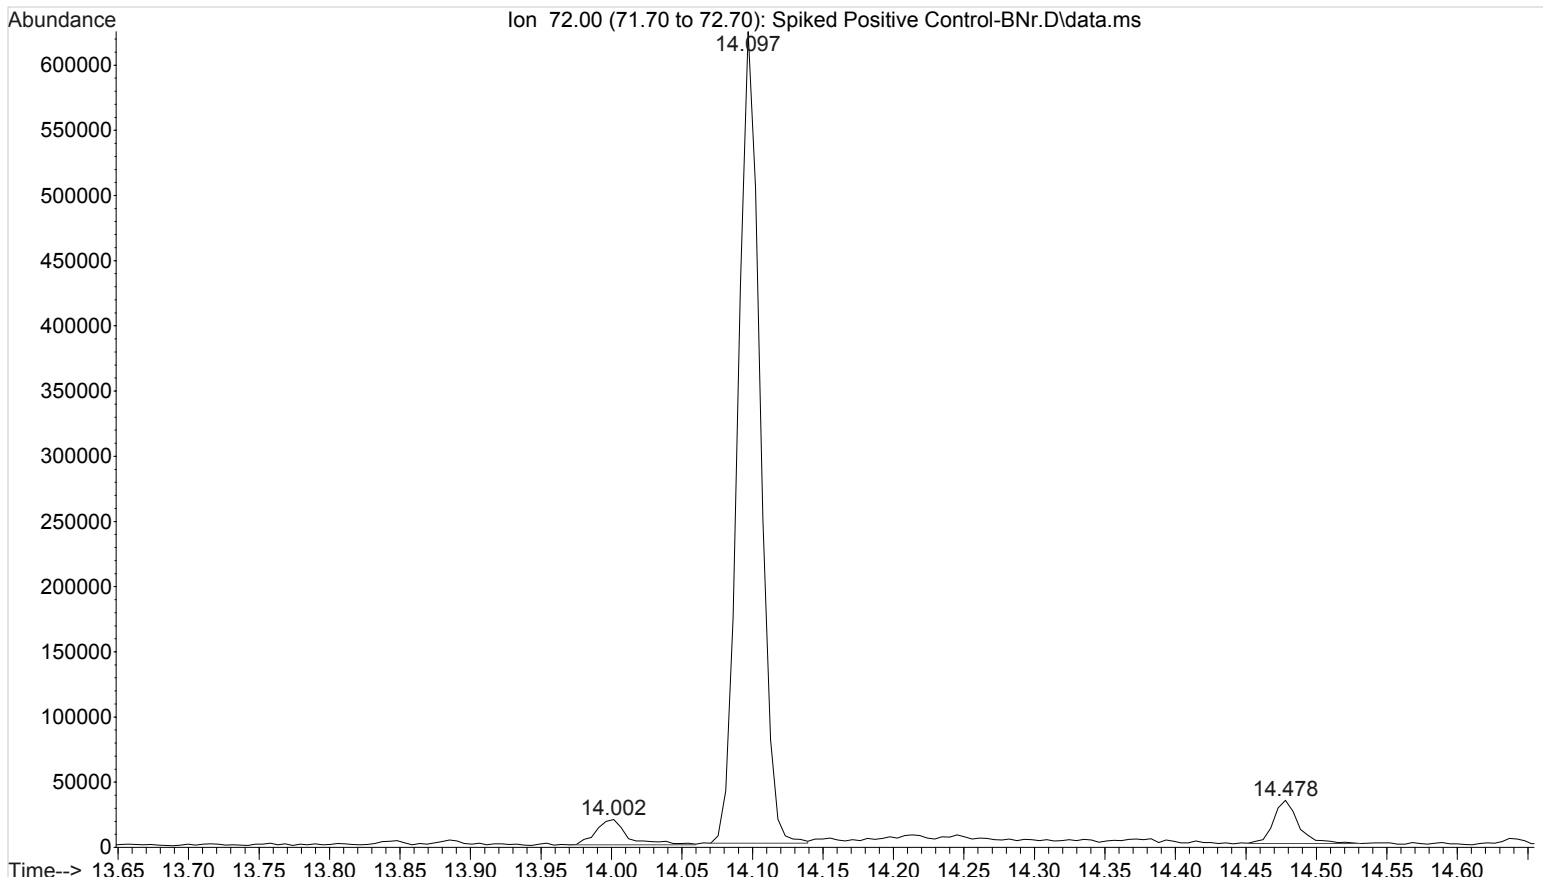

File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\080516  
... \Spiked Positive Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 05 Aug 2016 18:13 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

9

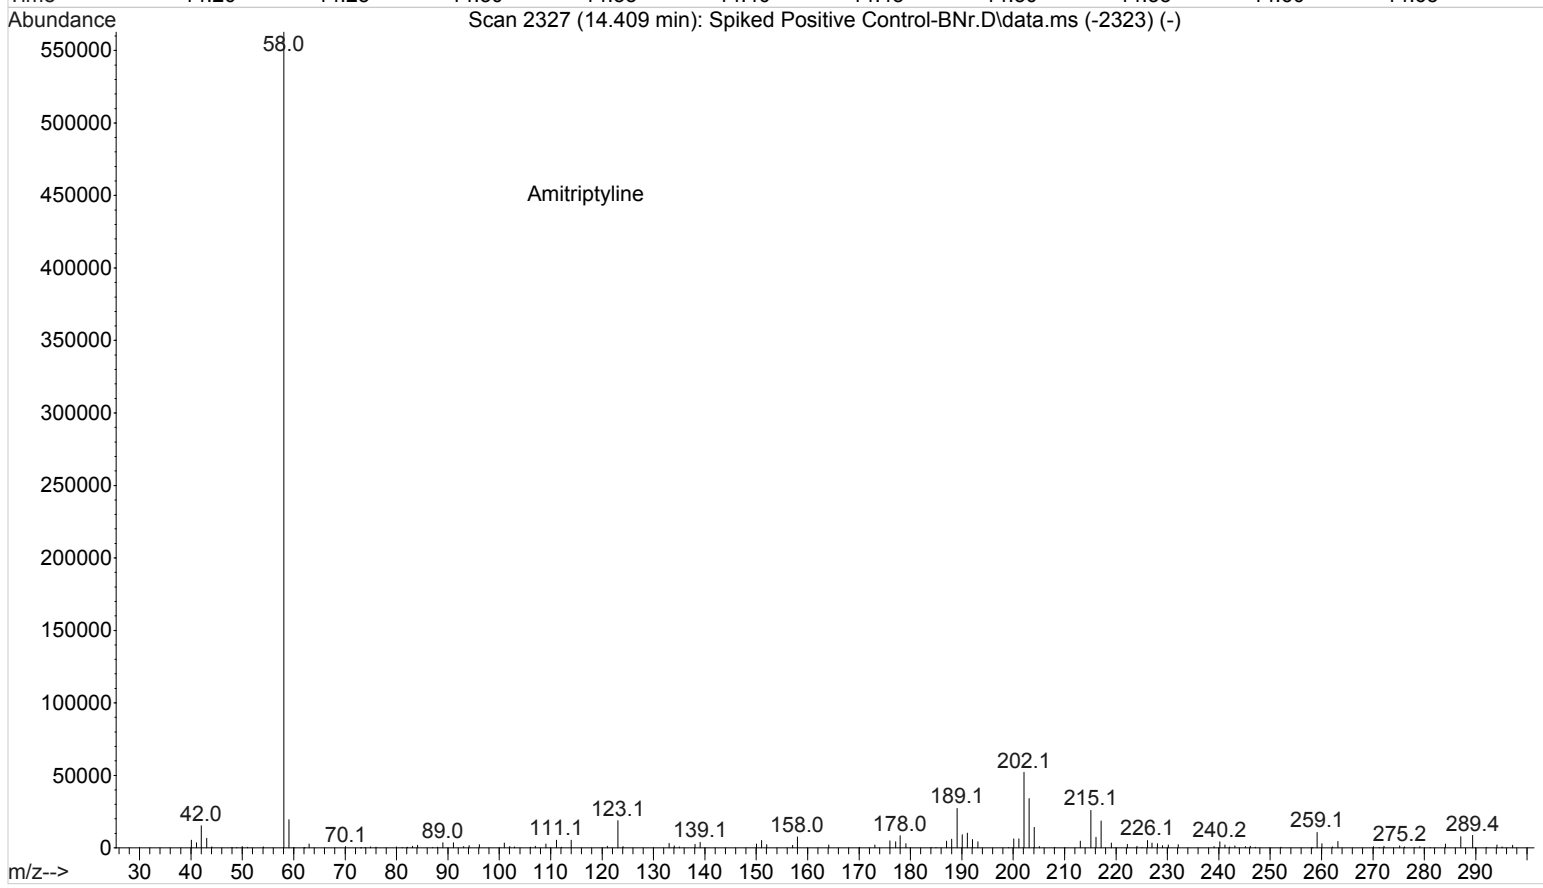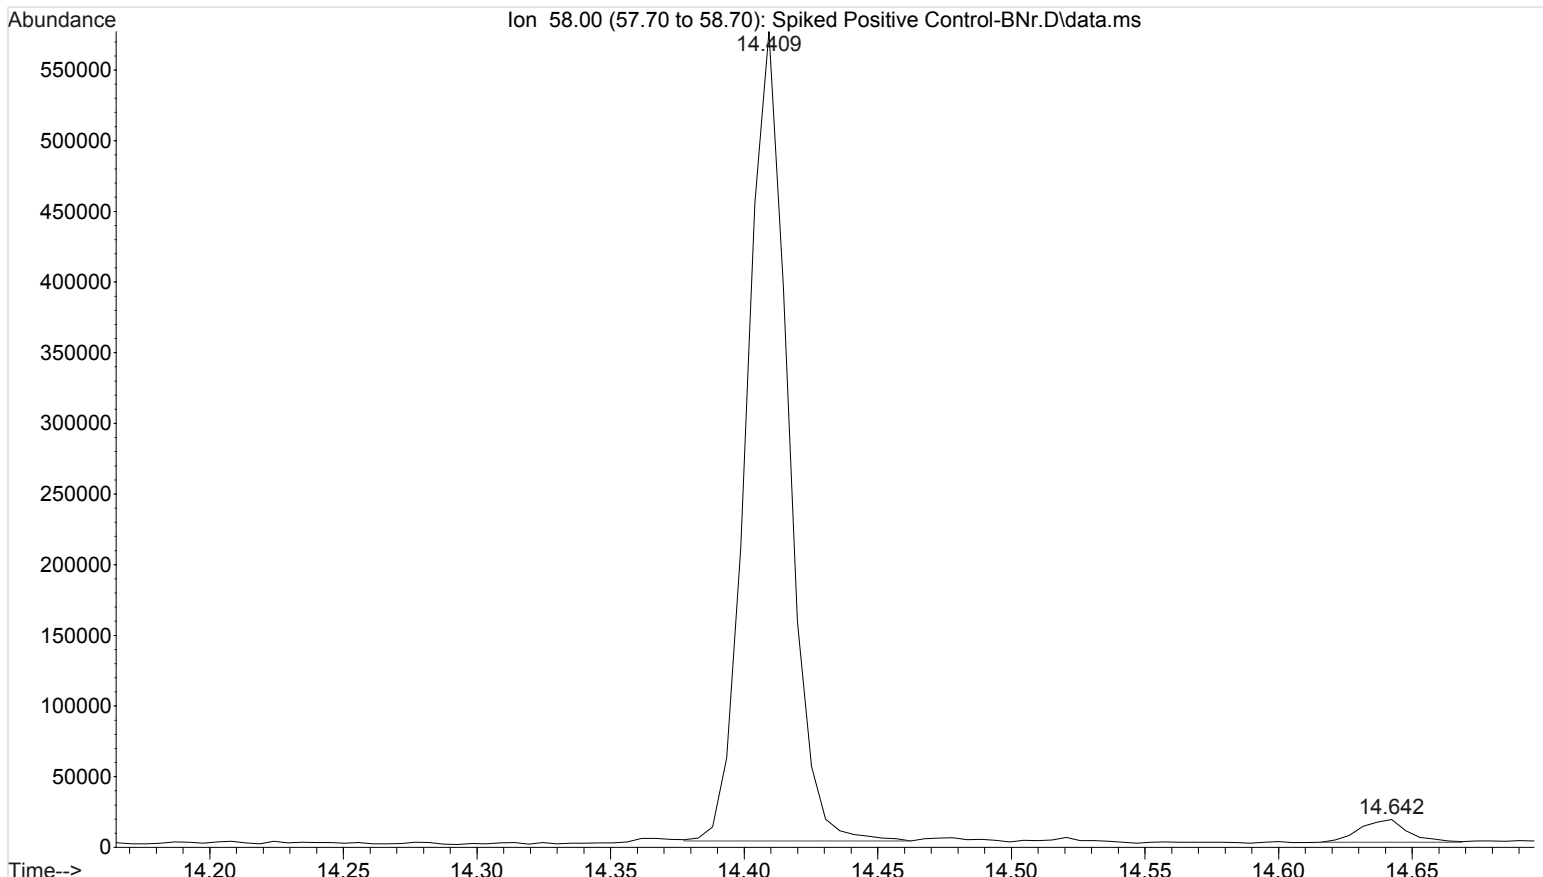

File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\080516  
... \Spiked Positive Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 05 Aug 2016 18:13 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

