
























Worklist: 1321

central data reviewed by B. Wylie on 10/27/16



10/20/2016

<u>LAB_CASE</u>	<u>ITEM</u>	<u>TASK_ID</u>	<u>DESCRIPTION</u>	
M2016-2481	2	58790	AM 8 Blood base neutral confir	
M2016-2546	2	59140	AM 8 Blood base neutral confir	
M2016-2561	1	66785	AM 8 Blood base neutral confir	
M2016-2678	3	59993	AM 8 Blood base neutral confir	
P2016-1240	1	57100	AM 8 Blood base neutral confir	
P2016-1251	1	57203	AM 8 Blood base neutral confir	
P2016-1258	8	57340	AM 8 Blood base neutral confir	
P2016-1260	1	57334	AM 8 Blood base neutral confir	
P2016-1261	1	57337	AM 8 Blood base neutral confir	
P2016-1262	1	57347	AM 8 Blood base neutral confir	
P2016-1263	1	57350	AM 8 Blood base neutral confir	
P2016-1296	1	59453	AM 8 Blood base neutral confir	
P2016-1302	1	57510	AM 8 Blood base neutral confir	
P2016-1326	1	57769	AM 8 Blood base neutral confir	
P2016-1328	1	57782	AM 8 Blood base neutral confir	
P2016-1331	1	57861	AM 8 Blood base neutral confir	
P2016-1336	1	57905	AM 8 Blood base neutral confir	
P2016-1363	1	58118	AM 8 Blood base neutral confir	
P2016-1364	1	58123	AM 8 Blood base neutral confir	
P2016-1373	1	58174	AM 8 Blood base neutral confir	
P2016-1374	2	58178	AM 8 Blood base neutral confir	
P2016-1380	1	58291	AM 8 Blood base neutral confir	
P2016-1443	1	58631	AM 8 Blood base neutral confir	

Worklist: 1321



<u>LAB CASE</u>	<u>ITEM</u>	<u>TASK ID</u>	<u>DESCRIPTION</u>
P2016-1457	1	58787	AM 8 Blood base neutral confir
P2016-1507	1	59013	AM 8 Blood base neutral confir



reviewed 11/1/16



Sequence verified *tm*
10/20/16

tm

simulate_sequence.log
Simulate Run Sequence Wed Oct 19 11:41:30 2016

Instrument Name: Major Mass Spec
Sequence File: C:\Users\ISPuser\Desktop\Sequences\tm-blanks.sequence.xml
Comment: MassHunter sequence
Operator: ISP\datastor
Data Path: D:\DATA\TM\2016\10192016\
Method Path: C:\Users\datastor\Desktop\OP Methods\

Line	Type	Vials	DataFile	Sample Name
Acquisition Method: BNSB120510.M				
1)	Sample	✓ 100	Prerun Solvent Blank	Pre-run Solvent Blank
2)	Sample	✓ 1	Negative Control-BN	Negative Control -
...1013				
3)	Sample	✓ 2	Spiked Positive Control-BN	Positive Control
4)	Sample	99	prbLK2	Solvent Blank
Acquisition Method: GBT092509-Delta EMV.M				
5)	Sample	100	Prerun Solvent Blankr	Pre-run Solvent Blank
6)	Sample	✓ 1	Negative Control-BNr	Negative Control -
...1013				
7)	Sample	✓ 2	Spiked Positive Control-BNr	Positive Control
8)	Sample	✓ 99	prbLK2r	Solvent Blank
Acquisition Method: BNSB120510.M				
9)	Sample	100	M2016-2481-2-BNBLK	Lab No.: M2016-2481-2
10)	Sample	✓ 3	M2016-2481-2-BN	Lab No.: M2016-2481-2
Acquisition Method: GBT092509-Delta EMV.M				
11)	Sample	✓ 3	M2016-2481-2-BNr	Lab No.: M2016-2481-2
Acquisition Method: BNSB120510.M				
12)	Sample	100	M2016-2546-2-BNBLK	Lab No.: M2016-2546-2
13)	Sample	✓ 4	M2016-2546-2-BN	Lab No.: M2016-2546-2
Acquisition Method: GBT092509-Delta EMV.M				
14)	Sample	✓ 4	M2016-2546-2-BNr	Lab No.: M2016-2546-2
Acquisition Method: BNSB120510.M				
15)	Sample	100	M2016-2561-1-BNBLK	Lab No.: M2016-2561-1
16)	Sample	✓ 5	M2016-2561-1-BN	Lab No.: M2016-2561-1
Acquisition Method: GBT092509-Delta EMV.M				
17)	Sample	✓ 5	M2016-2561-1-BNr	Lab No.: M2016-2561-1
Acquisition Method: BNSB120510.M				
18)	Sample	100	M2016-2678-3-BNBLK	Lab No.: M2016-2678-3
19)	Sample	✓ 6	M2016-2678-3-BN	Lab No.: M2016-2678-3
Acquisition Method: GBT092509-Delta EMV.M				
20)	Sample	✓ 6	M2016-2678-3-BNr	Lab No.: M2016-2678-3
Acquisition Method: BNSB120510.M				
21)	Sample	100	P2016-1240-1-BNBLK	Lab No.: P2016-1240-1
22)	Sample	✓ 7	P2016-1240-1-BN	Lab No.: P2016-1240-1
Acquisition Method: GBT092509-Delta EMV.M				
23)	Sample	✓ 7	P2016-1240-1-BNr	Lab No.: P2016-1240-1
Acquisition Method: BNSB120510.M				
24)	Sample	100	P2016-1251-1-BNBLK	Lab No.: P2016-1251-1
25)	Sample	✓ 8	P2016-1251-1-BN	Lab No.: P2016-1251-1
Acquisition Method: GBT092509-Delta EMV.M				
26)	Sample	✓ 8	P2016-1251-1-BNr	Lab No.: P2016-1251-1

simulate_sequence.log

Acquisition Method:	BNSB120510.M		
27) Sample	100	P2016-1258-8-BNBLK	Lab No.: P2016-1258-8
28) Sample	✓9	P2016-1258-8-BN	Lab No.: P2016-1258-8
Acquisition Method:	GBT092509-Delta EMV.M		
29) Sample	✓9	P2016-1258-8-BNr	Lab No.: P2016-1258-8
Acquisition Method:	BNSB120510.M		
30) Sample	100	P2016-1260-1-BNBLK	Lab No.: P2016-1260-1
31) Sample	✓10	P2016-1260-1-BN	Lab No.: P2016-1260-1
Acquisition Method:	GBT092509-Delta EMV.M		
32) Sample	✓10	P2016-1260-1-BNr	Lab No.: P2016-1260-1
Acquisition Method:	BNSB120510.M		
33) Sample	100	P2016-1261-1-BNBLK	Lab No.: P2016-1261-1
34) Sample	✓11	P2016-1261-1-BN	Lab No.: P2016-1261-1
Acquisition Method:	GBT092509-Delta EMV.M		
35) Sample	✓11	P2016-1261-1-BNr	Lab No.: P2016-1261-1
Acquisition Method:	BNSB120510.M		
36) Sample	100	P2016-1262-1-BNBLK	Lab No.: P2016-1262-1
37) Sample	✓12	P2016-1262-1-BN	Lab No.: P2016-1262-1
Acquisition Method:	GBT092509-Delta EMV.M		
38) Sample	✓12	P2016-1262-1-BNr	Lab No.: P2016-1262-1
Acquisition Method:	BNSB120510.M		
39) Sample	100	P2016-1263-1-BNBLK	Lab No.: P2016-1263-1
40) Sample	✓13	P2016-1263-1-BN	Lab No.: P2016-1263-1
Acquisition Method:	GBT092509-Delta EMV.M		
41) Sample	✓13	P2016-1263-1-BNr	Lab No.: P2016-1263-1
Acquisition Method:	BNSB120510.M		
42) Sample	100	P2016-1296-1-BNBLK	Lab No.: P2016-1296-1
43) Sample	✓14	P2016-1296-1-BN	Lab No.: P2016-1296-1
Acquisition Method:	GBT092509-Delta EMV.M		
44) Sample	✓14	P2016-1296-1-BNr	Lab No.: P2016-1296-1
Acquisition Method:	BNSB120510.M		
45) Sample	100	P2016-1302-1-BNBLK	Lab No.: P2016-1302-1
46) Sample	✓15	P2016-1302-1-BN	Lab No.: P2016-1302-1
Acquisition Method:	GBT092509-Delta EMV.M		
47) Sample	✓15	P2016-1302-1-BNr	Lab No.: P2016-1302-1
Acquisition Method:	BNSB120510.M		
48) Sample	✓99	P2016-1326-1-BNBLK	Lab No.: P2016-1326-1
49) Sample	✓16	P2016-1326-1-BN	Lab No.: P2016-1326-1
Acquisition Method:	GBT092509-Delta EMV.M		
50) Sample	✓16	P2016-1326-1-BNr	Lab No.: P2016-1326-1
Acquisition Method:	BNSB120510.M		
51) Sample	✓99	P2016-1328-1-BNBLK	Lab No.: P2016-1328-1
52) Sample	✓17	P2016-1328-1-BN	Lab No.: P2016-1328-1
Acquisition Method:	GBT092509-Delta EMV.M		
53) Sample	✓17	P2016-1328-1-BNr	Lab No.: P2016-1328-1
Acquisition Method:	BNSB120510.M		
54) Sample	✓99	P2016-1331-1-BNBLK	Lab No.: P2016-1331-1
55) Sample	✓18	P2016-1331-1-BN	Lab No.: P2016-1331-1

simulate_sequence.log

Acquisition Method: GBT092509-Delta EMV.M		
56) Sample	✓18 P2016-1331-1-BNr	Lab No.: P2016-1331-1
Acquisition Method: BNSB120510.M		
57) Sample	✓99 P2016-1336-1-BNBLK	Lab No.: P2016-1336-1
58) Sample	✓19 P2016-1336-1-BN	Lab No.: P2016-1336-1
Acquisition Method: GBT092509-Delta EMV.M		
59) Sample	✓19 P2016-1336-1-BNr	Lab No.: P2016-1336-1
Acquisition Method: BNSB120510.M		
60) Sample	✓99 P2016-1363-1-BNBLK	Lab No.: P2016-1363-1
61) Sample	✓20 P2016-1363-1-BN	Lab No.: P2016-1363-1
Acquisition Method: GBT092509-Delta EMV.M		
62) Sample	✓20 P2016-1363-1-BNr	Lab No.: P2016-1363-1
Acquisition Method: BNSB120510.M		
63) Sample	✓99 P2016-1364-1-BNBLK	Lab No.: P2016-1364-1
64) Sample	✓21 P2016-1364-1-BN	Lab No.: P2016-1364-1
Acquisition Method: GBT092509-Delta EMV.M		
65) Sample	✓21 P2016-1364-1-BNr	Lab No.: P2016-1364-1
Acquisition Method: BNSB120510.M		
66) Sample	✓99 P2016-1373-1-BNBLK	Lab No.: P2016-1373-1
67) Sample	✓22 P2016-1373-1-BN	Lab No.: P2016-1373-1
Acquisition Method: GBT092509-Delta EMV.M		
68) Sample	✓22 P2016-1373-1-BNr	Lab No.: P2016-1373-1
Acquisition Method: BNSB120510.M		
69) Sample	✓99 P2016-1374-1-BNBLK	Lab No.: P2016-1374-1
70) Sample	✓23 P2016-1374-1-BN	Lab No.: P2016-1374-1
Acquisition Method: GBT092509-Delta EMV.M		
71) Sample	✓23 P2016-1374-1-BNr	Lab No.: P2016-1374-1
Acquisition Method: BNSB120510.M		
72) Sample	✓99 P2016-1380-1-BNBLK	Lab No.: P2016-1380-1
73) Sample	✓24 P2016-1380-1-BN	Lab No.: P2016-1380-1
Acquisition Method: GBT092509-Delta EMV.M		
74) Sample	✓24 P2016-1380-1-BNr	Lab No.: P2016-1380-1
Acquisition Method: BNSB120510.M		
75) Sample	✓99 P2016-1443-1-BNBLK	Lab No.: P2016-1443-1
76) Sample	✓25 P2016-1443-1-BN	Lab No.: P2016-1443-1
Acquisition Method: GBT092509-Delta EMV.M		
77) Sample	✓25 P2016-1443-1-BNr	Lab No.: P2016-1443-1
Acquisition Method: BNSB120510.M		
78) Sample	✓99 P2016-1457-1-BNBLK	Lab No.: P2016-1457-1
79) Sample	✓26 P2016-1457-1-BN	Lab No.: P2016-1457-1
Acquisition Method: GBT092509-Delta EMV.M		
80) Sample	✓26 P2016-1457-1-BNr	Lab No.: P2016-1457-1
Acquisition Method: BNSB120510.M		
81) Sample	✓99 P2016-1507-1-BNBLK	Lab No.: P2016-1507-1
82) Sample	✓27 P2016-1507-1-BN	Lab No.: P2016-1507-1
Acquisition Method: GBT092509-Delta EMV.M		
83) Sample	✓27 P2016-1507-1-BNr	Lab No.: P2016-1507-1
Acquisition Method: BNSB120510.M		
84) Sample	✓99 POSTBLK	BLK


simulate_sequence.log

Acquisition Method: GBT092509-Delta EMV.M
85) Sample ✓99 AFTER
megabytes Needed: 844 Space on drive D: 216108
Sequence Verification Done!

BLK


Handwritten signature

File :F:\10192016\Prerun Solvent Blank.D
Operator : ISP\datastor
Acquired : 19 Oct 2016 11:44 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Pre-run Solvent Blank
Misc Info : Chloroform
Vial Number: 100

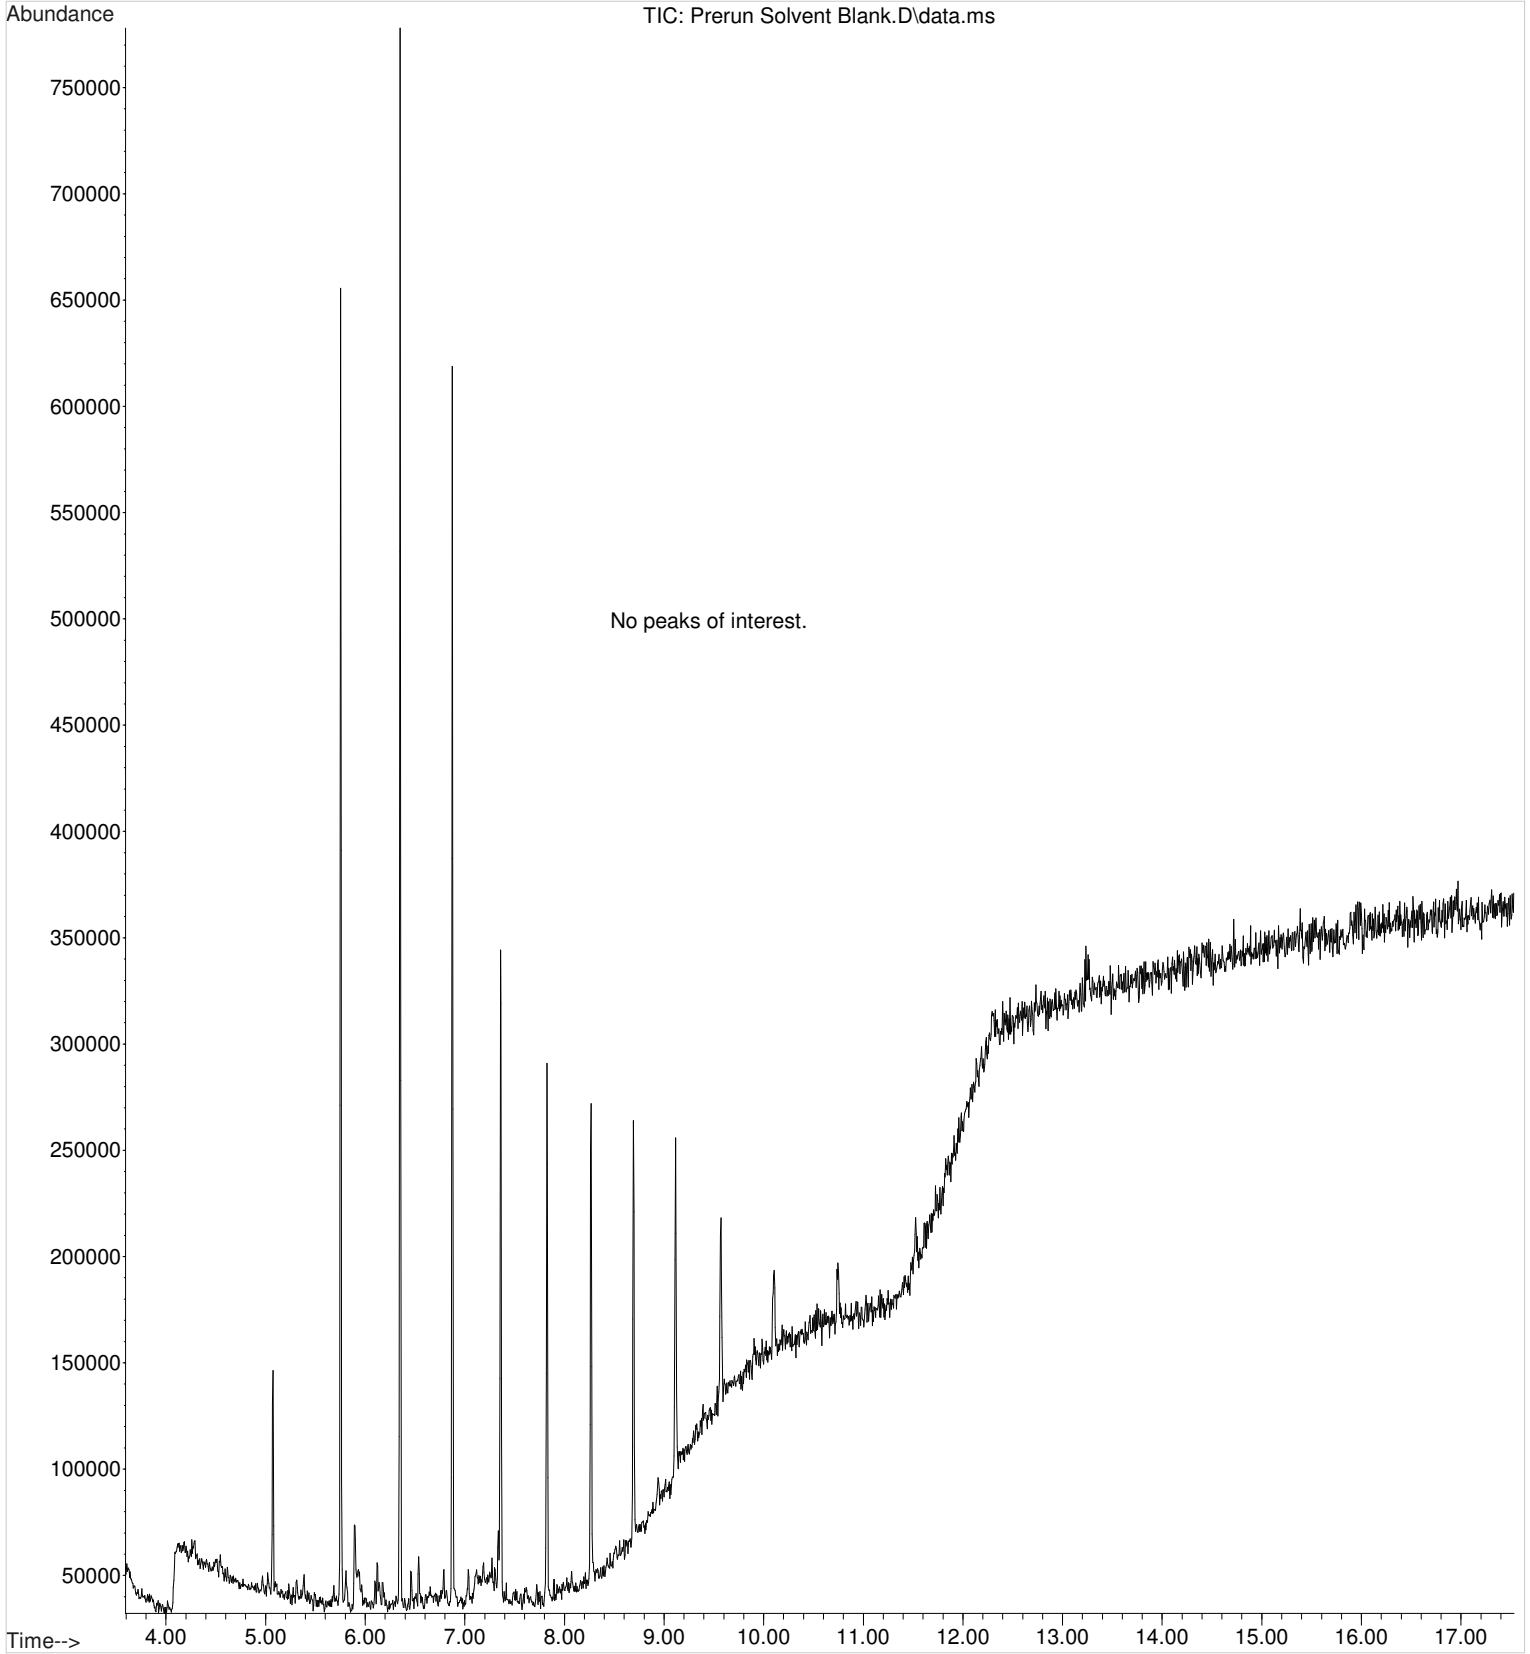


Handwritten signature

File :F:\10192016\prbLK2.D
Operator : ISP\datastor
Acquired : 19 Oct 2016 12:53 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Solvent Blank
Misc Info : Chloroform
Vial Number: 99


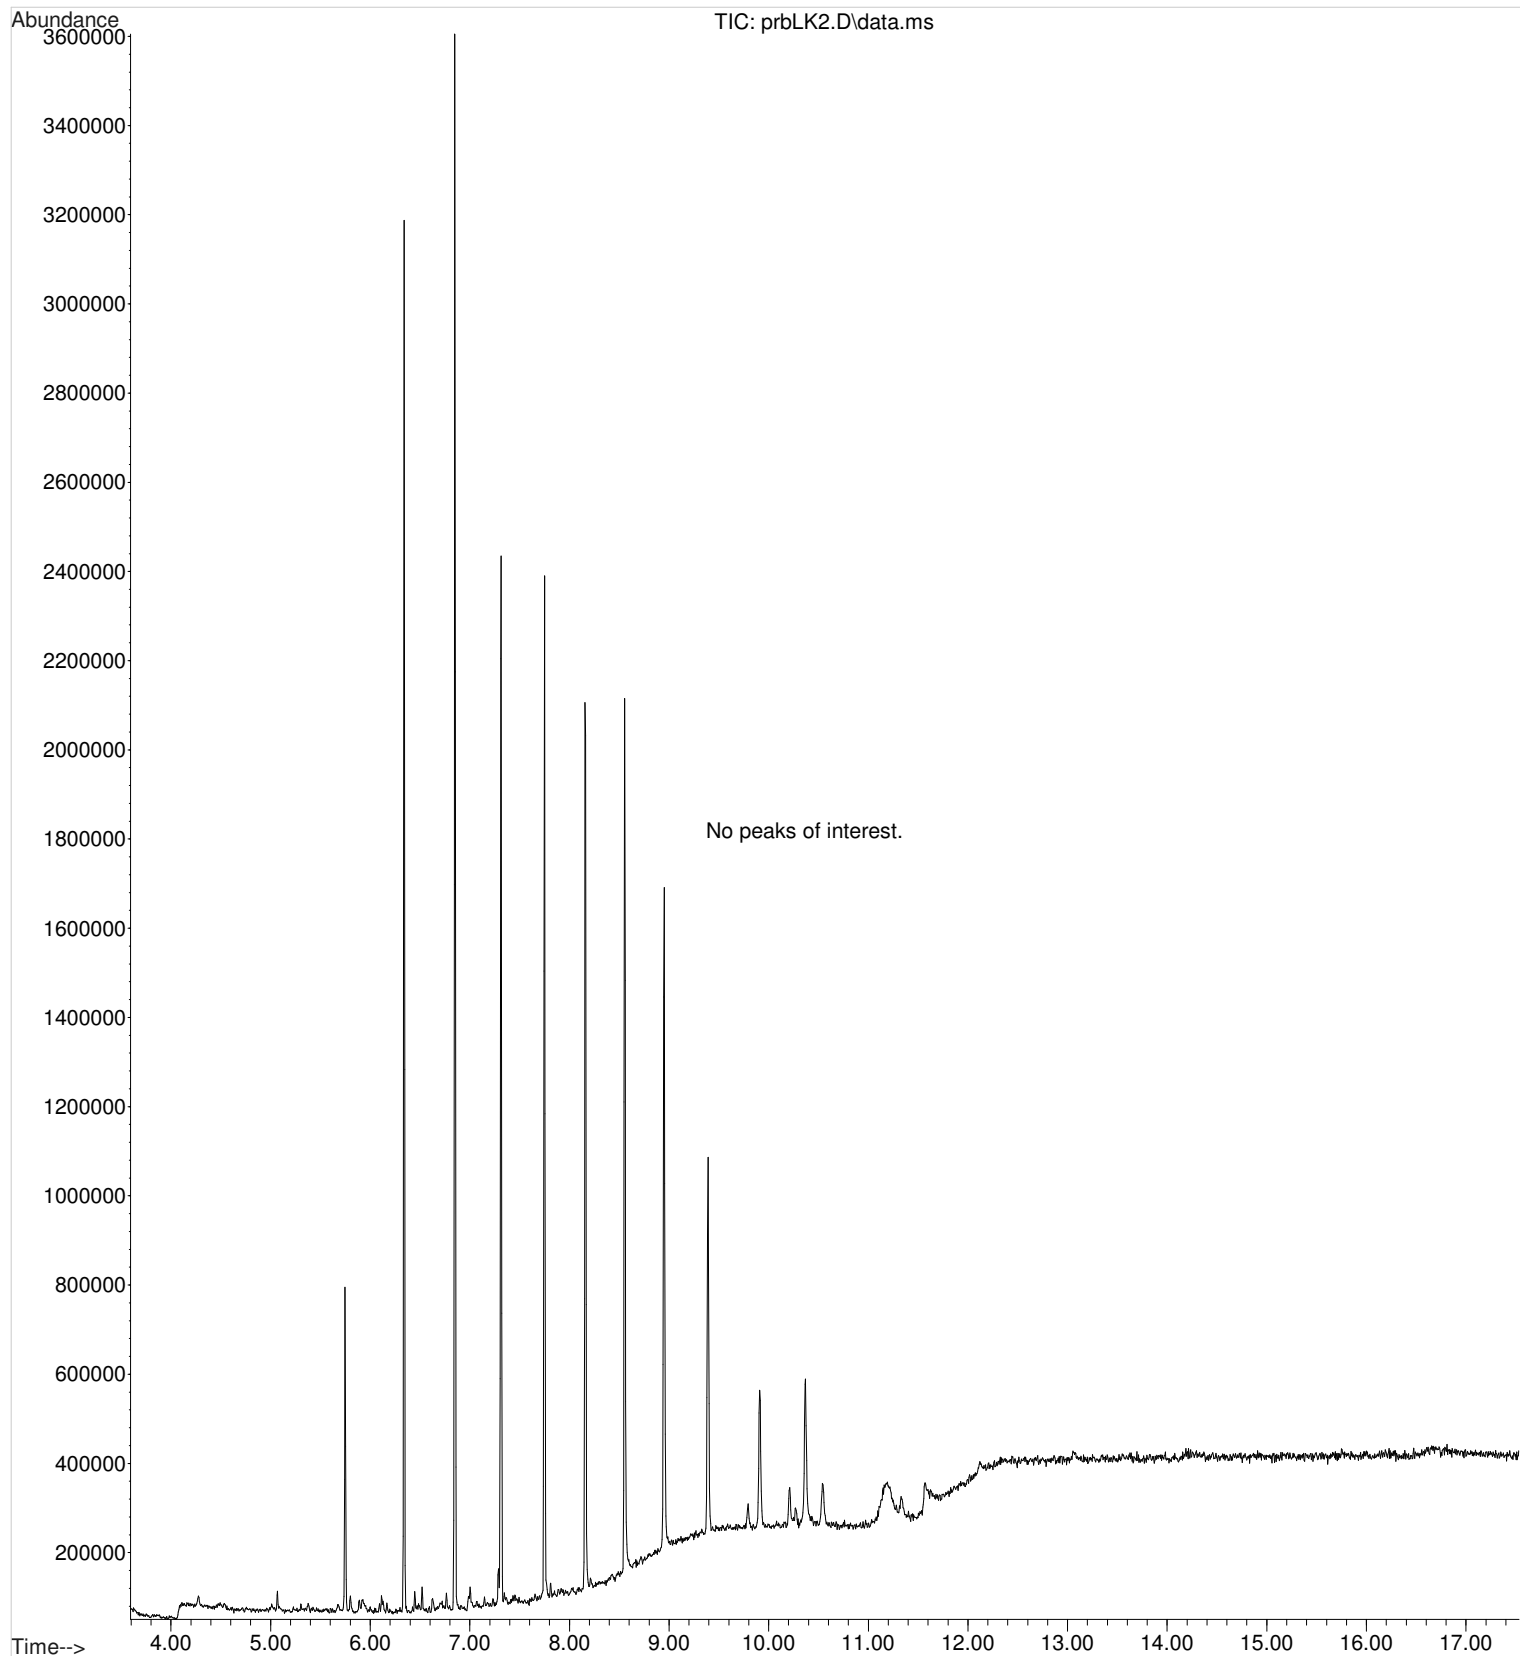


Handwritten signature



File :F:\10192016\Negative Control-BN.D
Operator : ISP\datastor
Acquired : 19 Oct 2016 12:07 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B1013
Misc Info : Analytical Method 3.6.1
Vial Number: 1

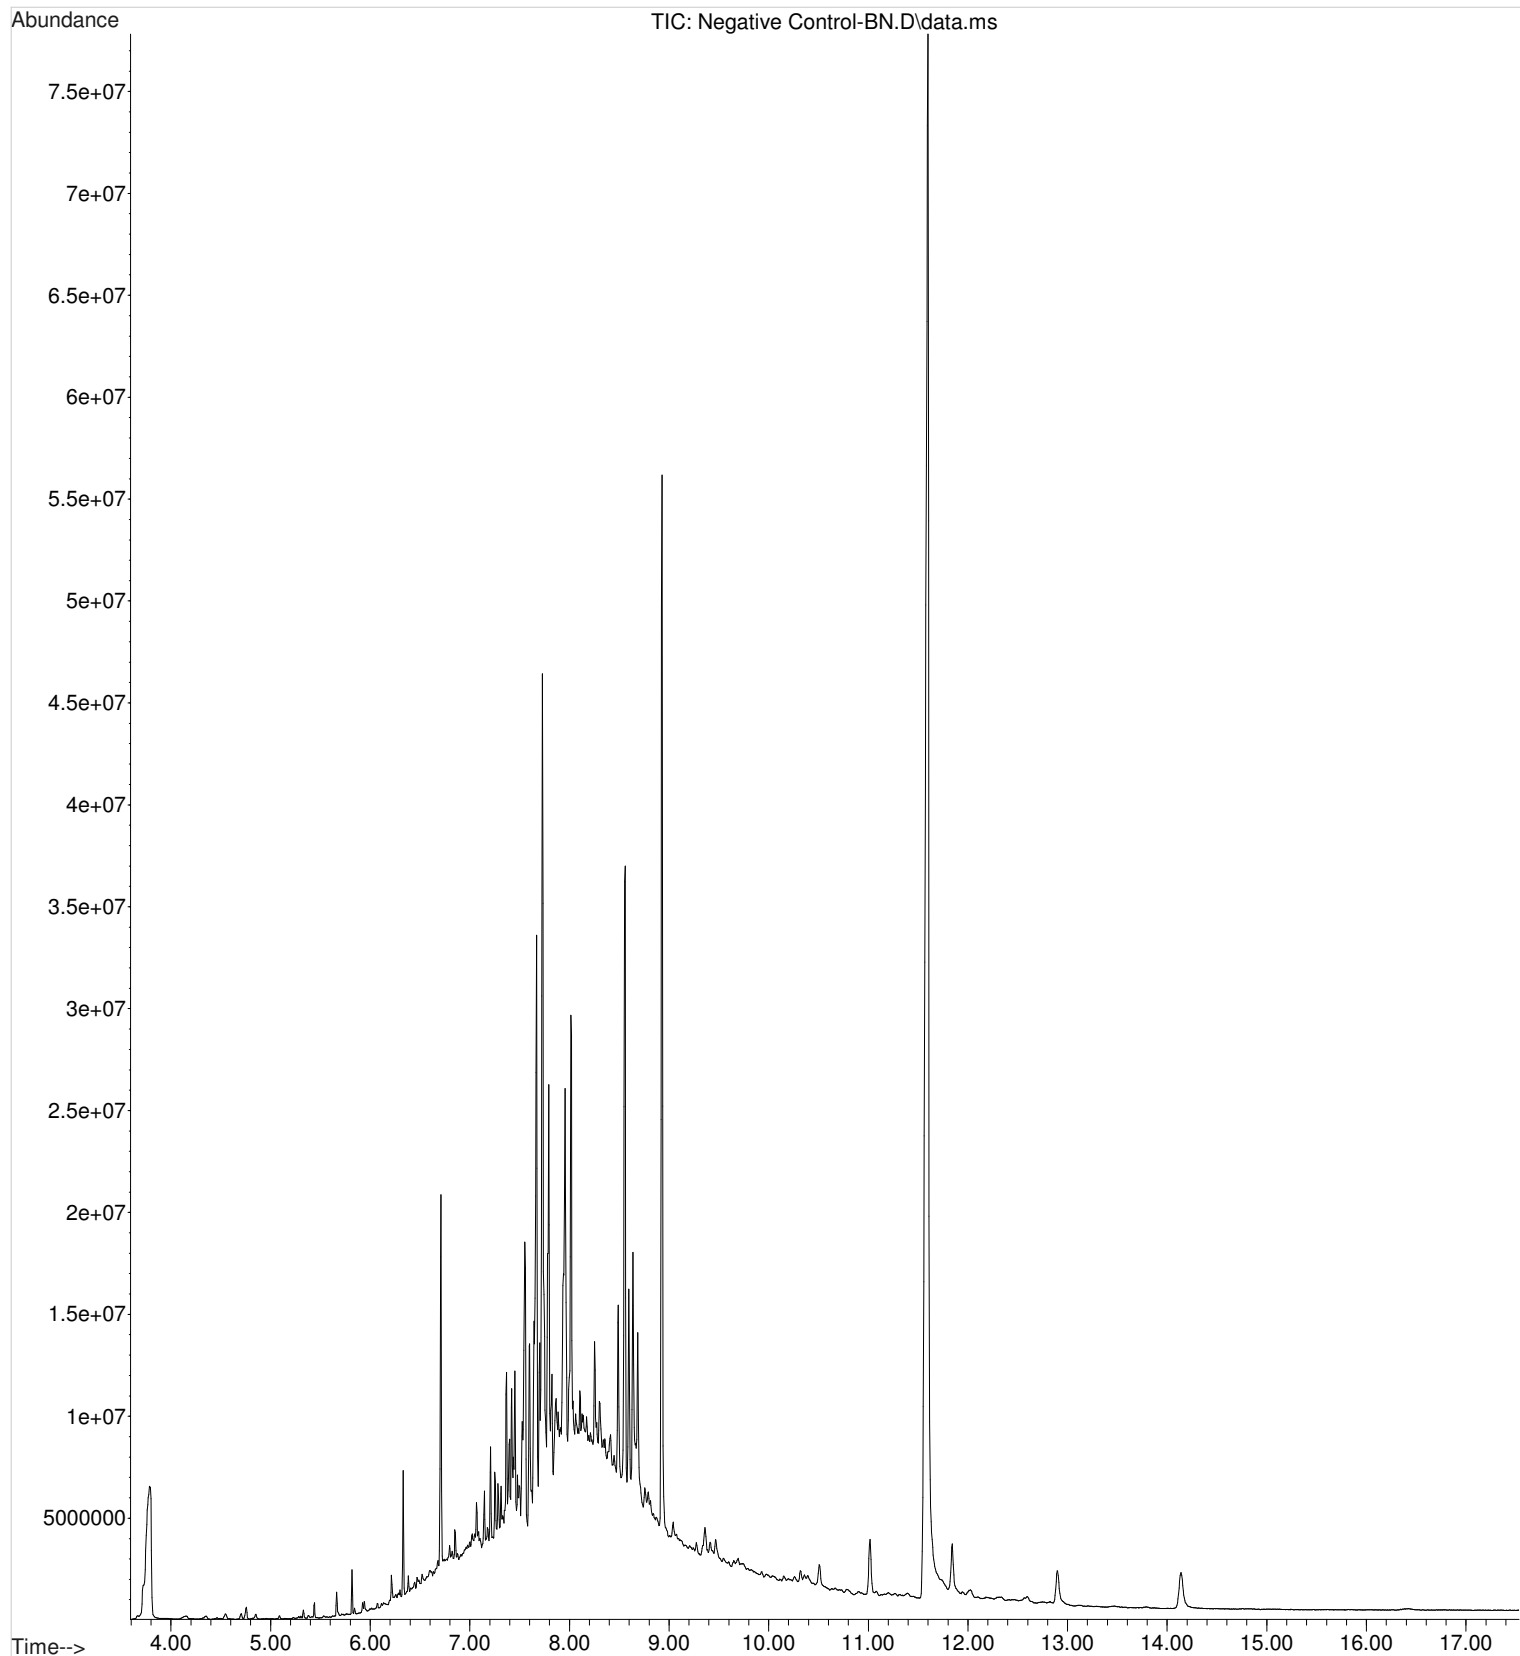


File : F:\10192016\Negative Control-BN.D
Operator : ISP\datastor
Acquired : 19 Oct 2016 12:07 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B1013
Misc Info : Analytical Method 3.6.1
Vial Number: 1

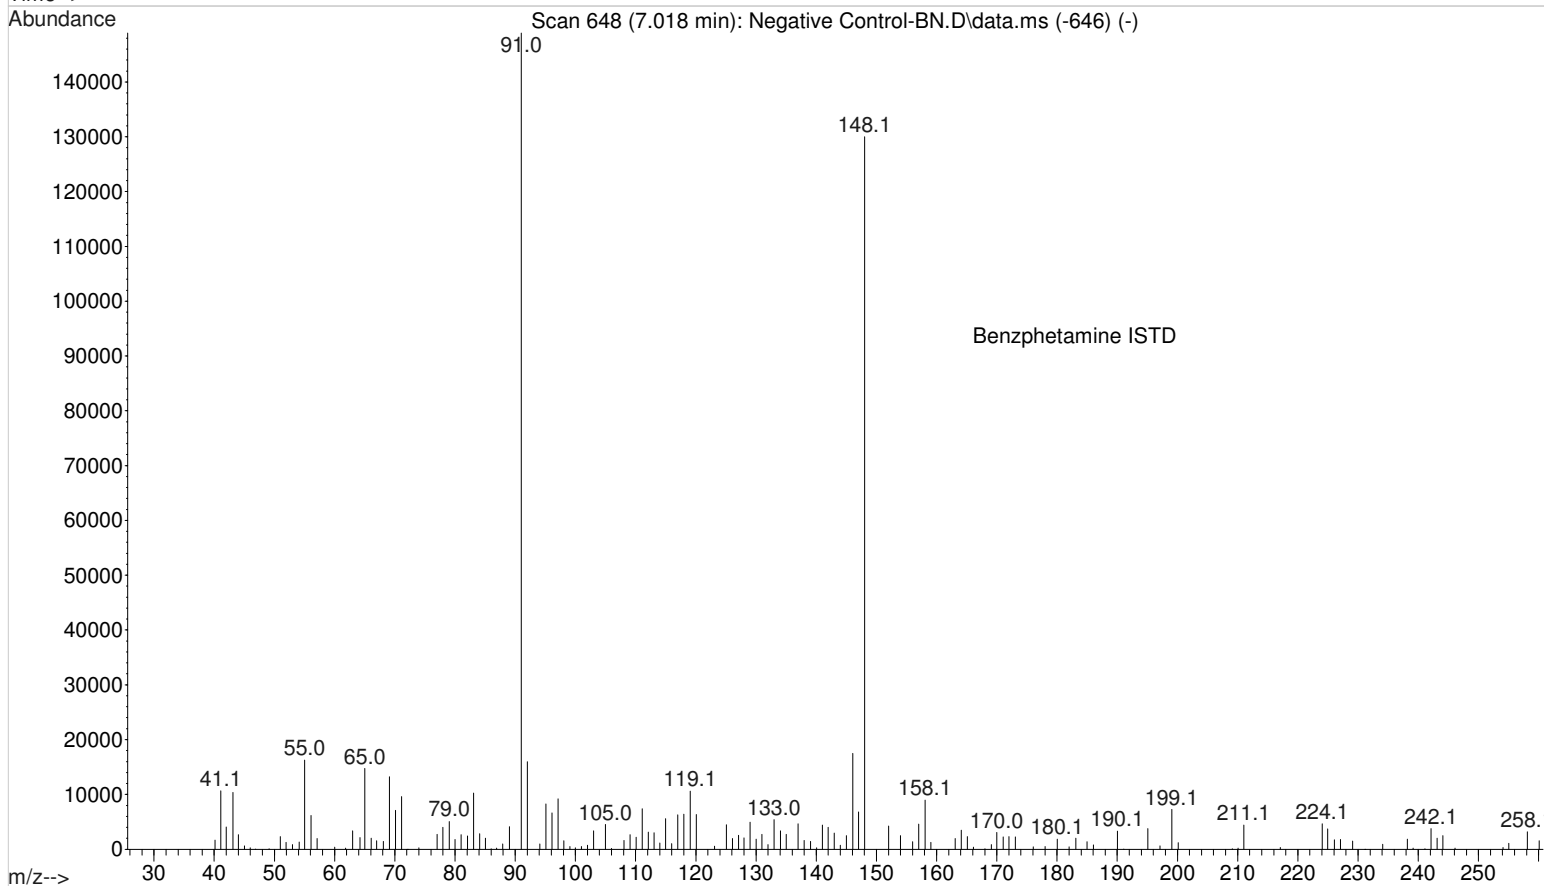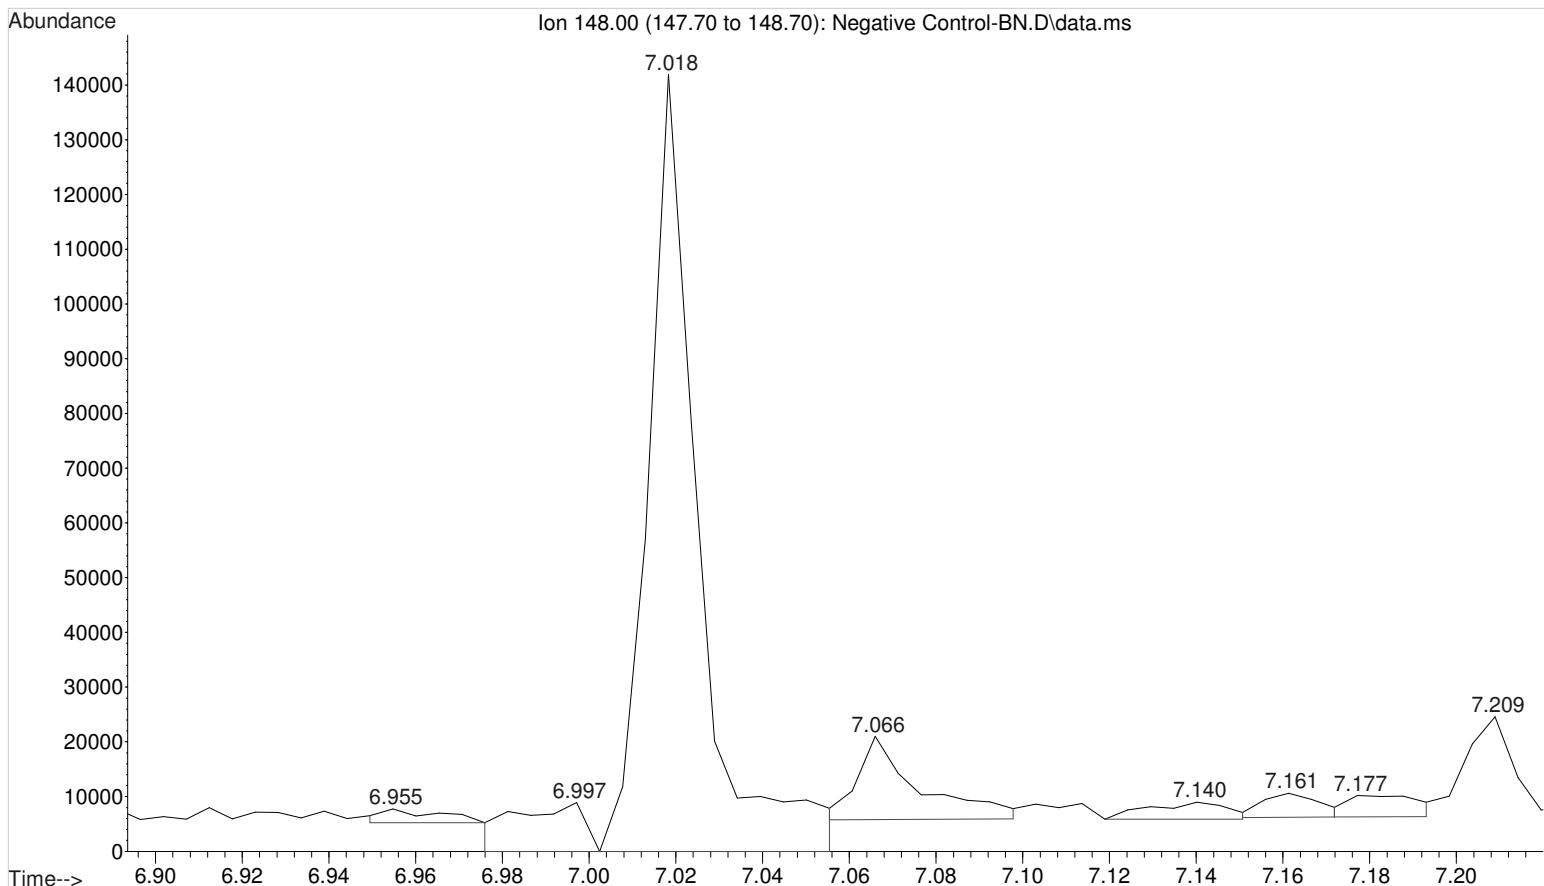



File :F:\10192016\Negative Control-BN.D
Operator : ISP\datastor
Acquired : 19 Oct 2016 12:07 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name : Negative Control - Utak Lot B1013
Misc Info : Analytical Method 3.6.1
Vial Number: 1

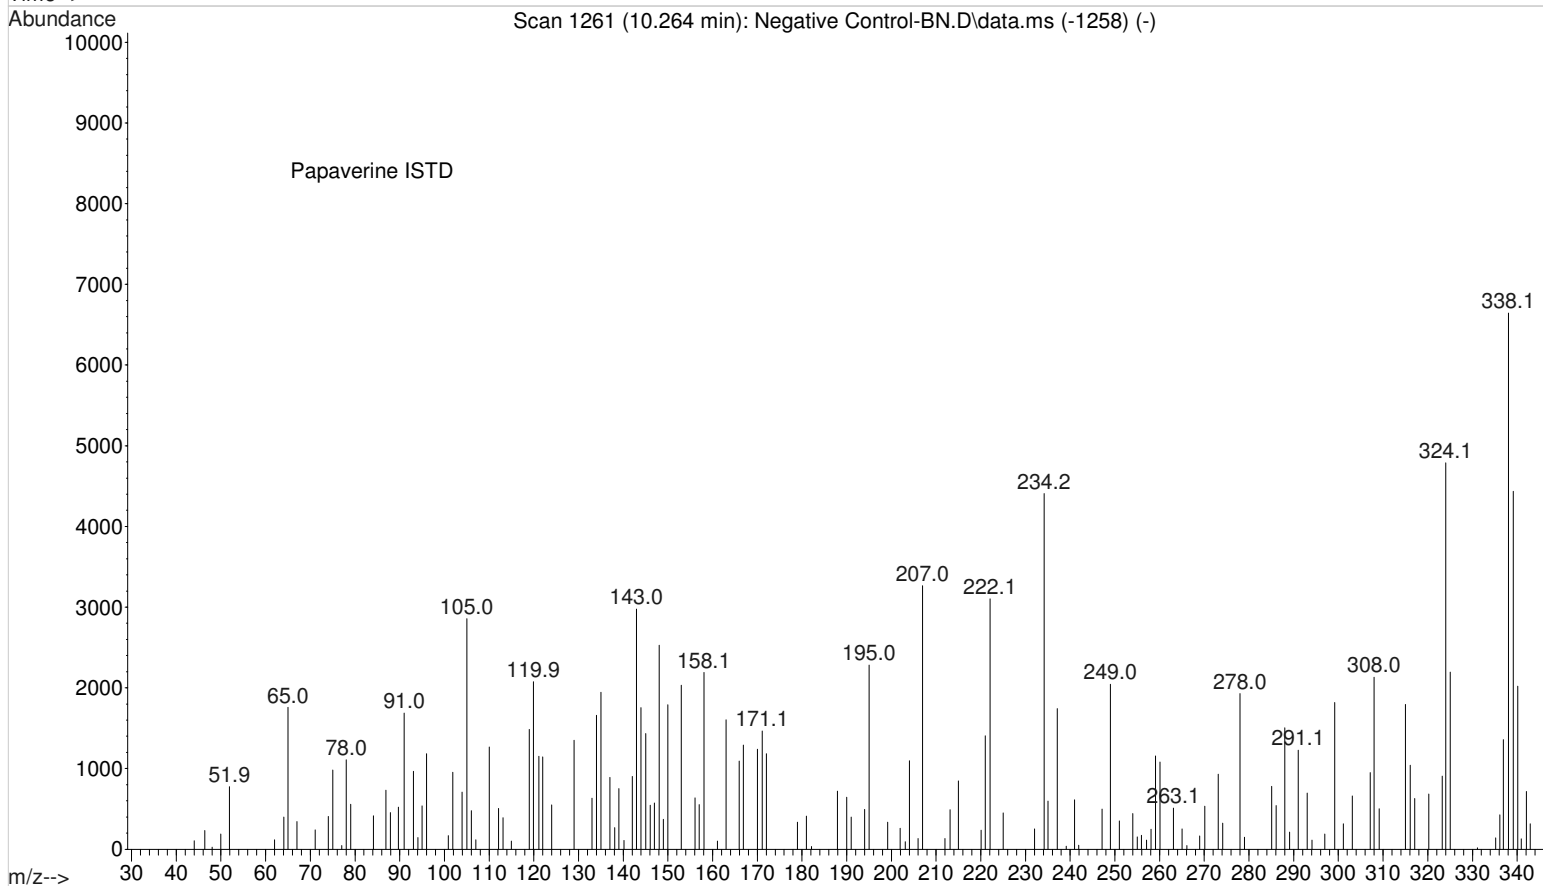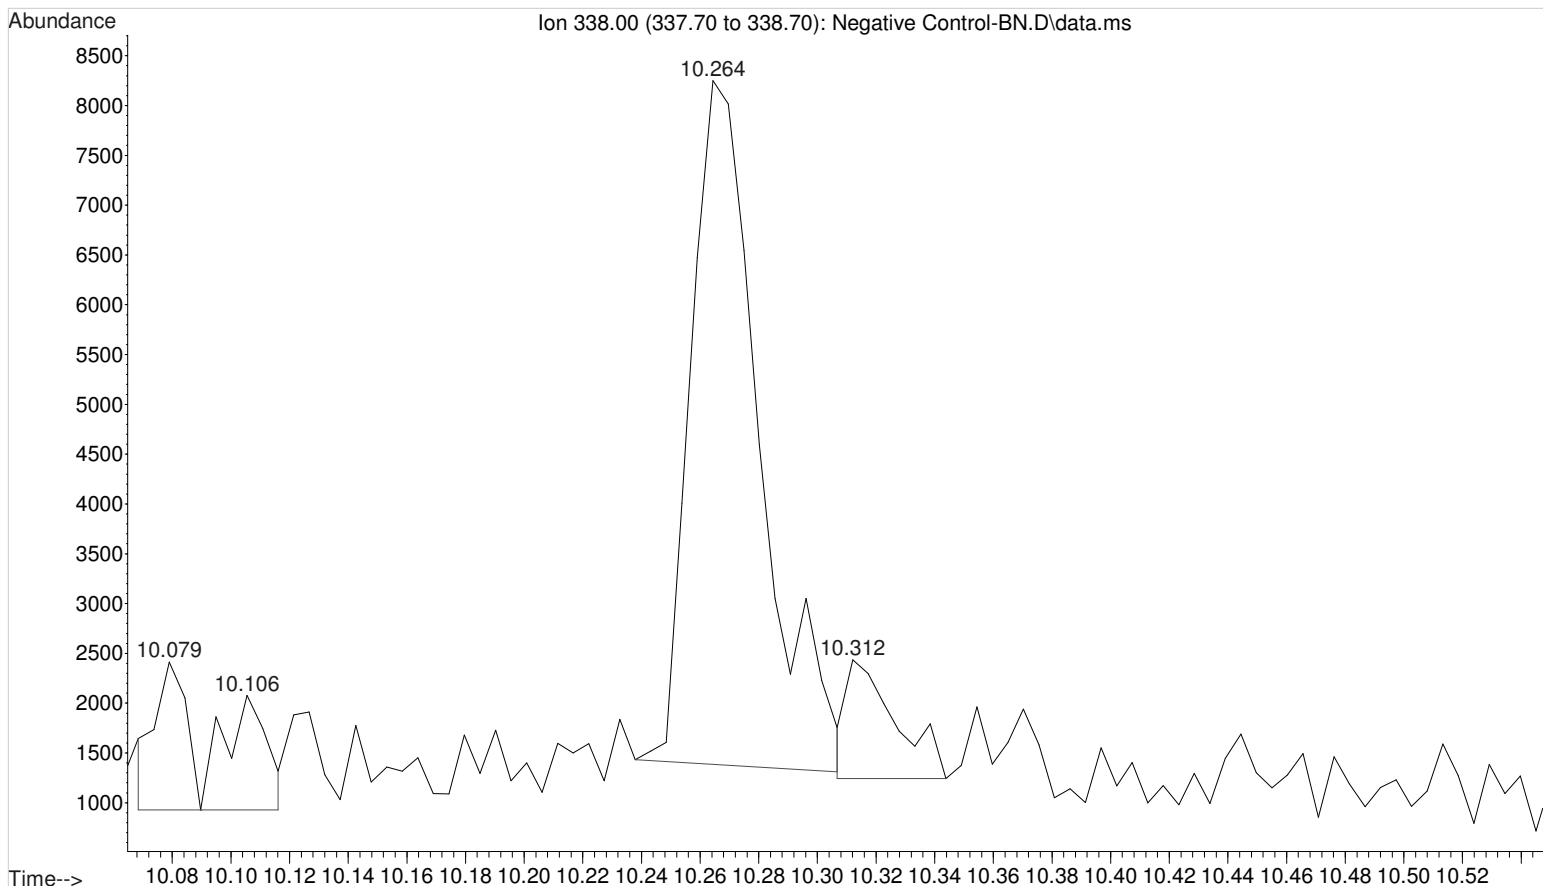



File : F:\10192016\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 19 Oct 2016 12:30 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

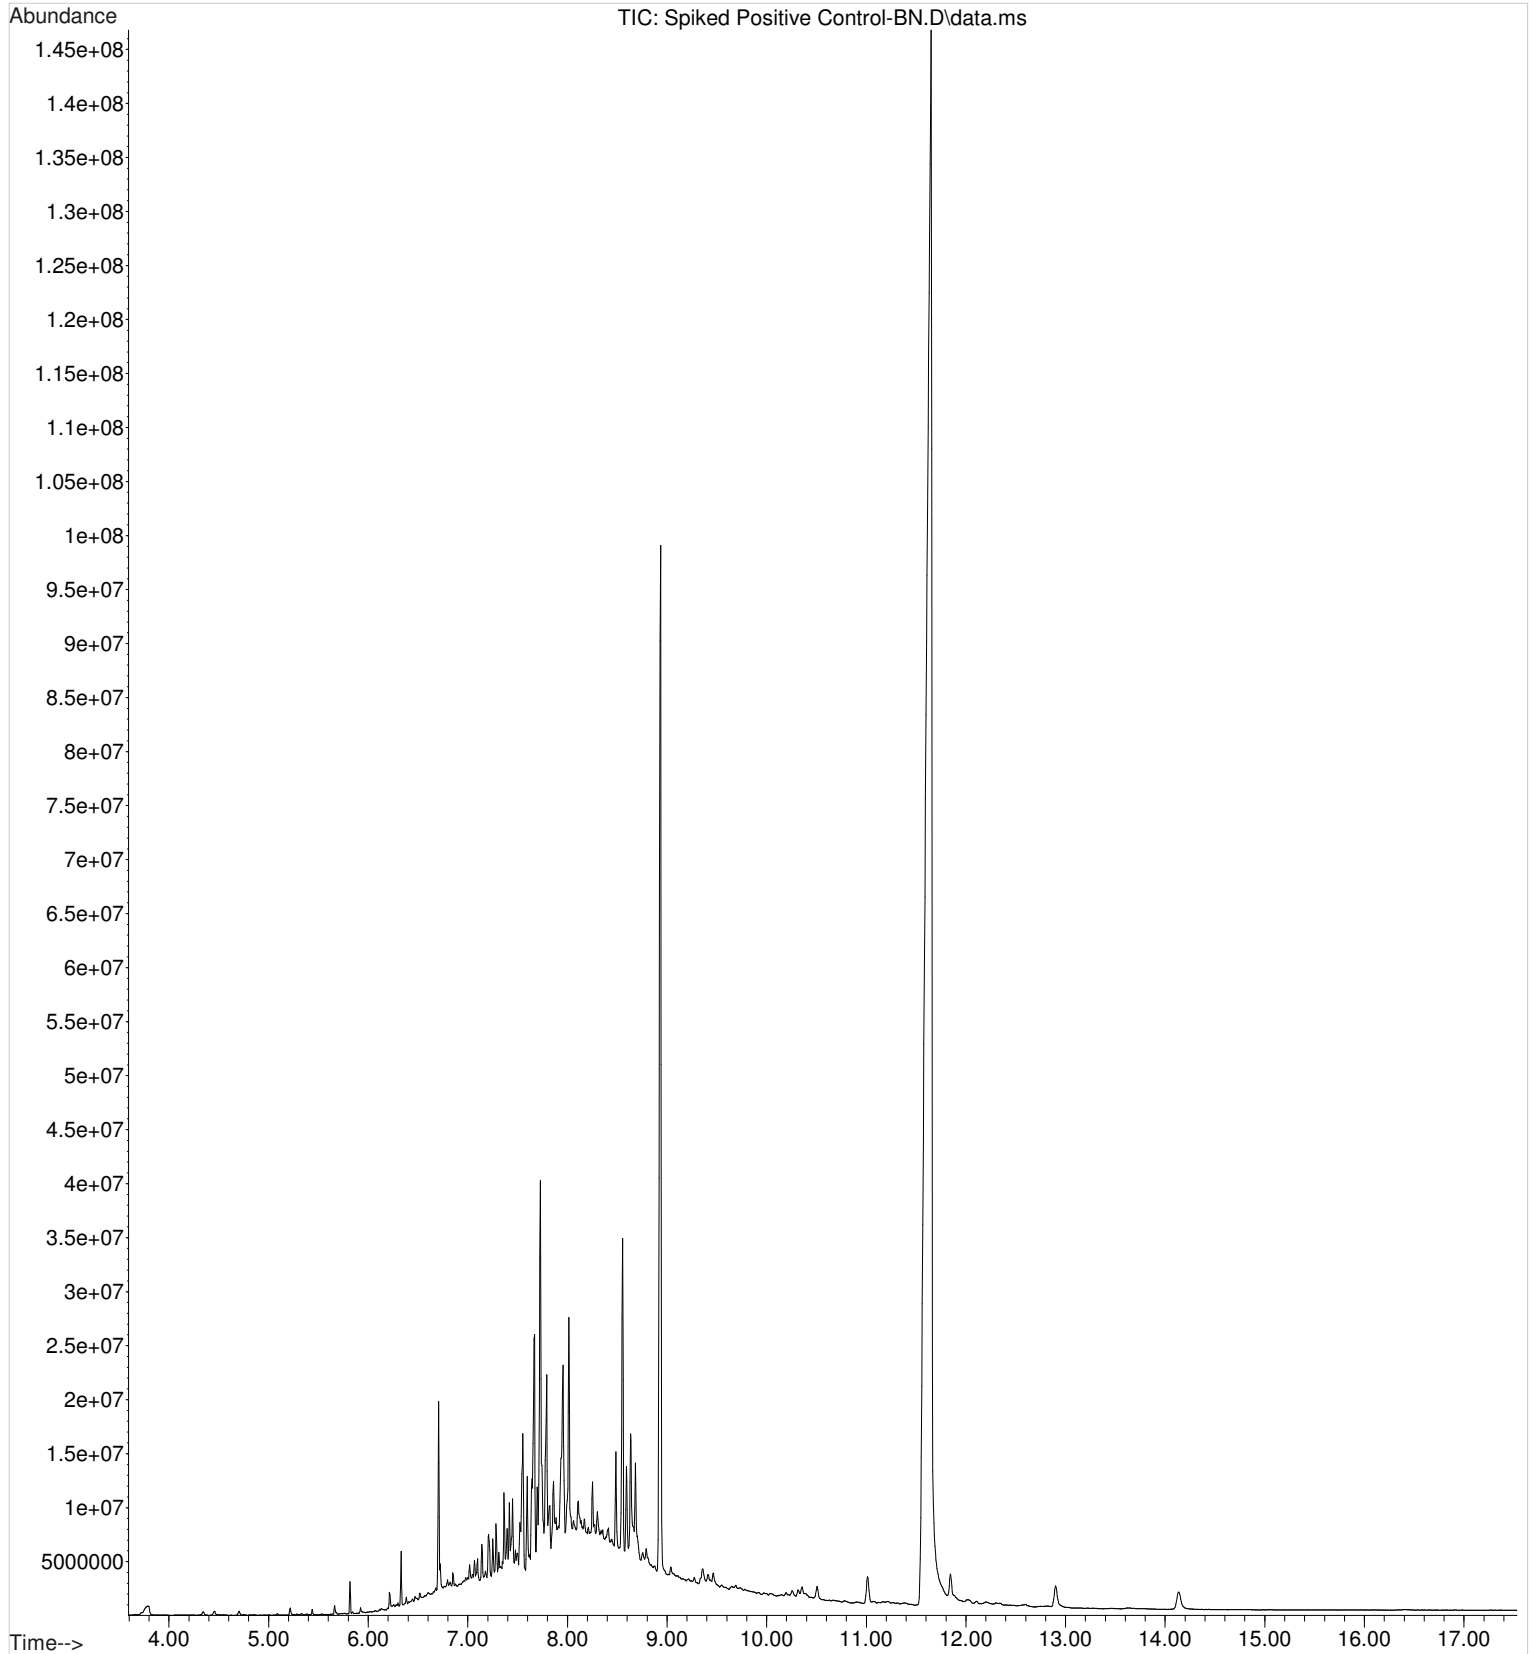



File : F:\10192016\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 19 Oct 2016 12:30 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

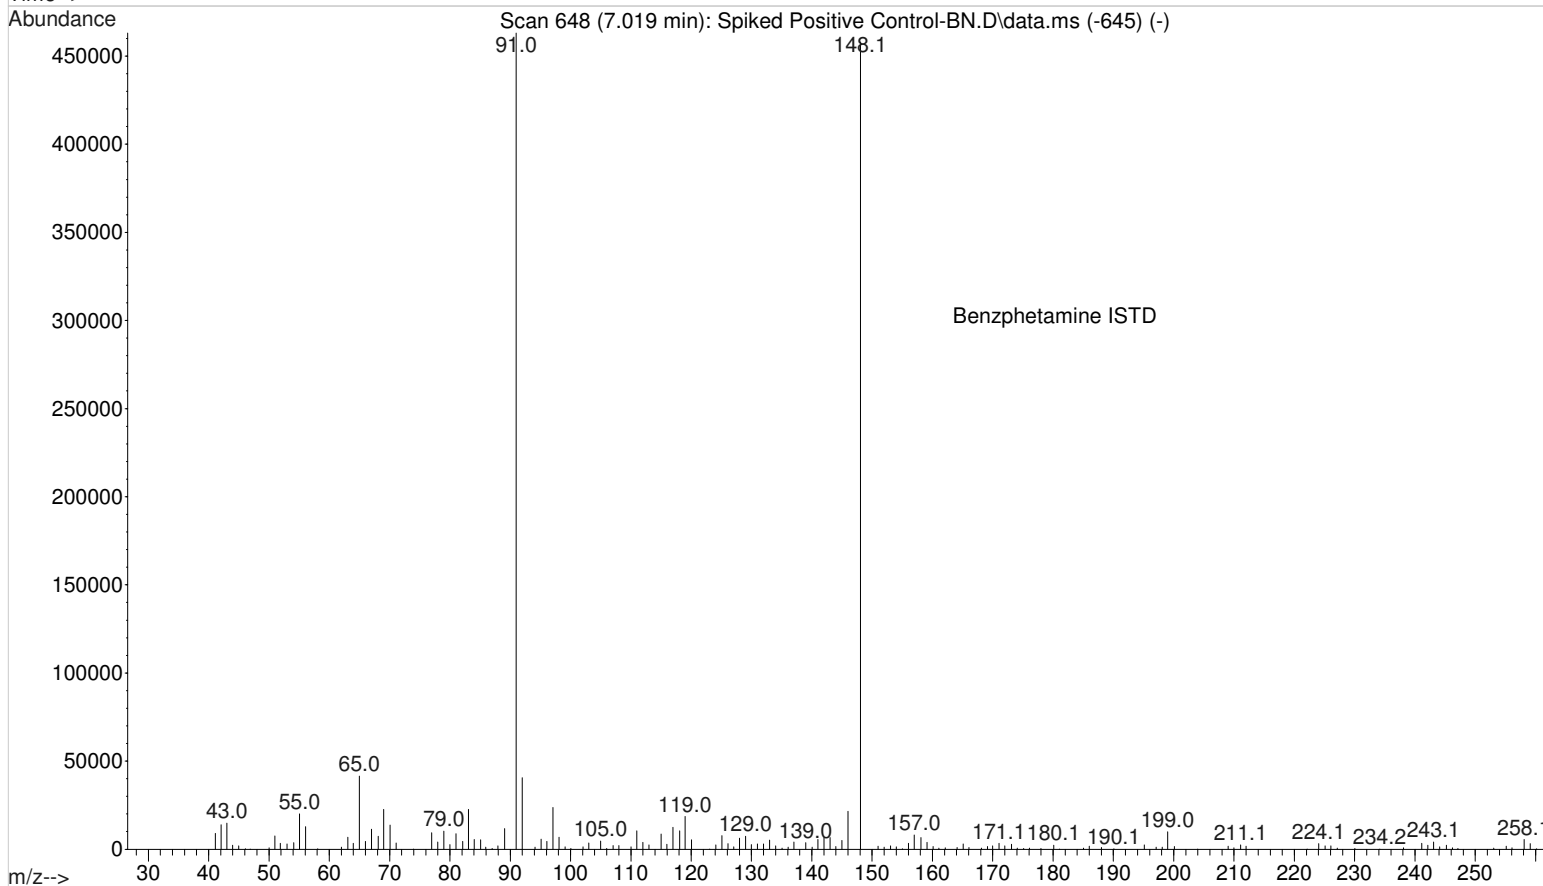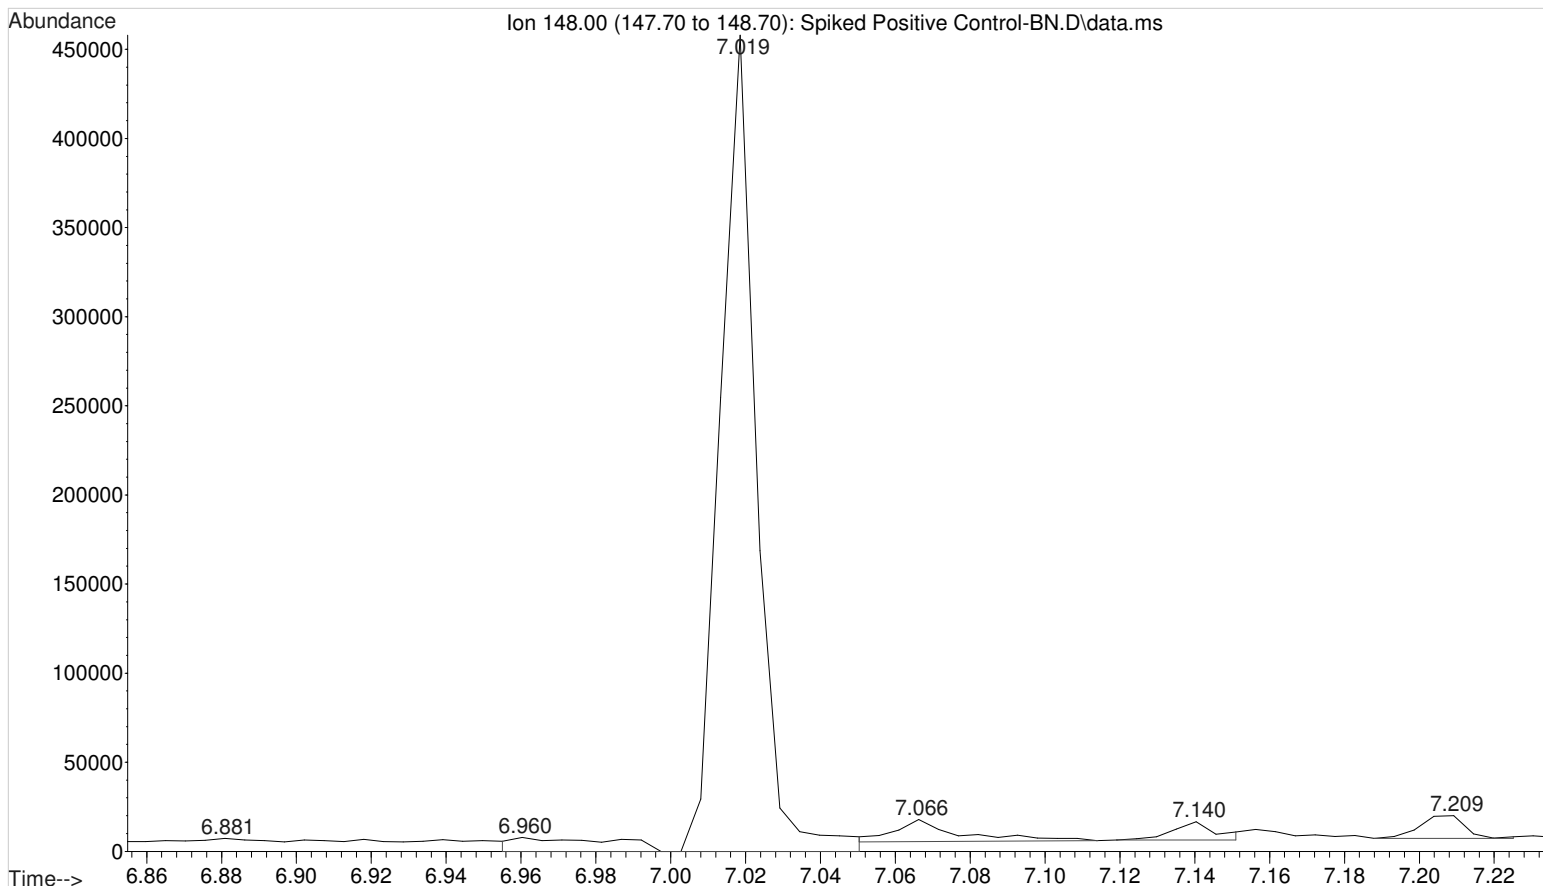



File : F:\10192016\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 19 Oct 2016 12:30 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name : Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

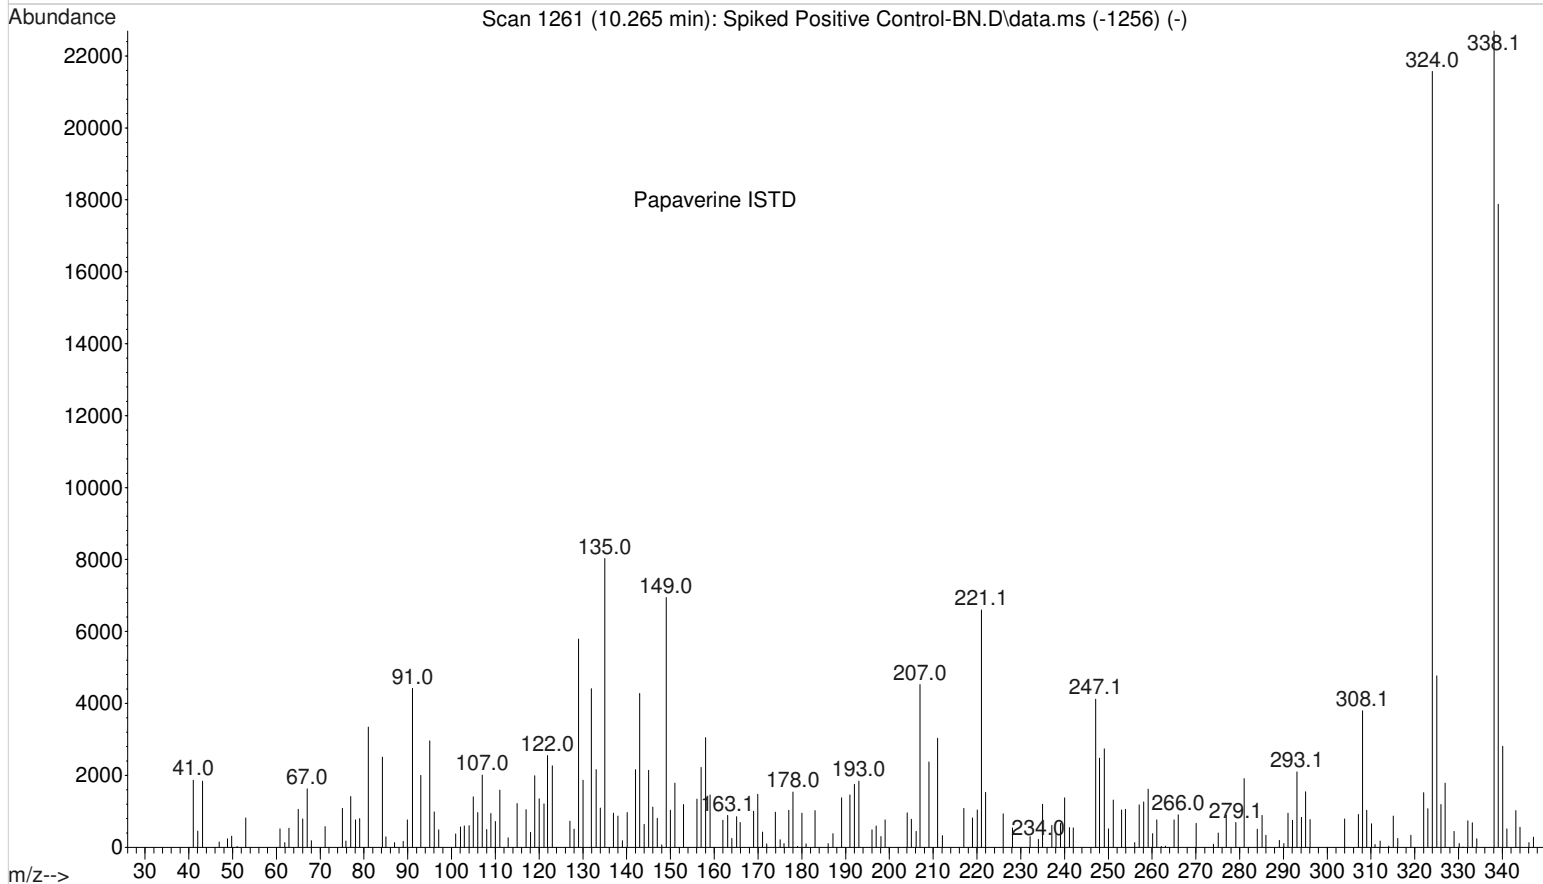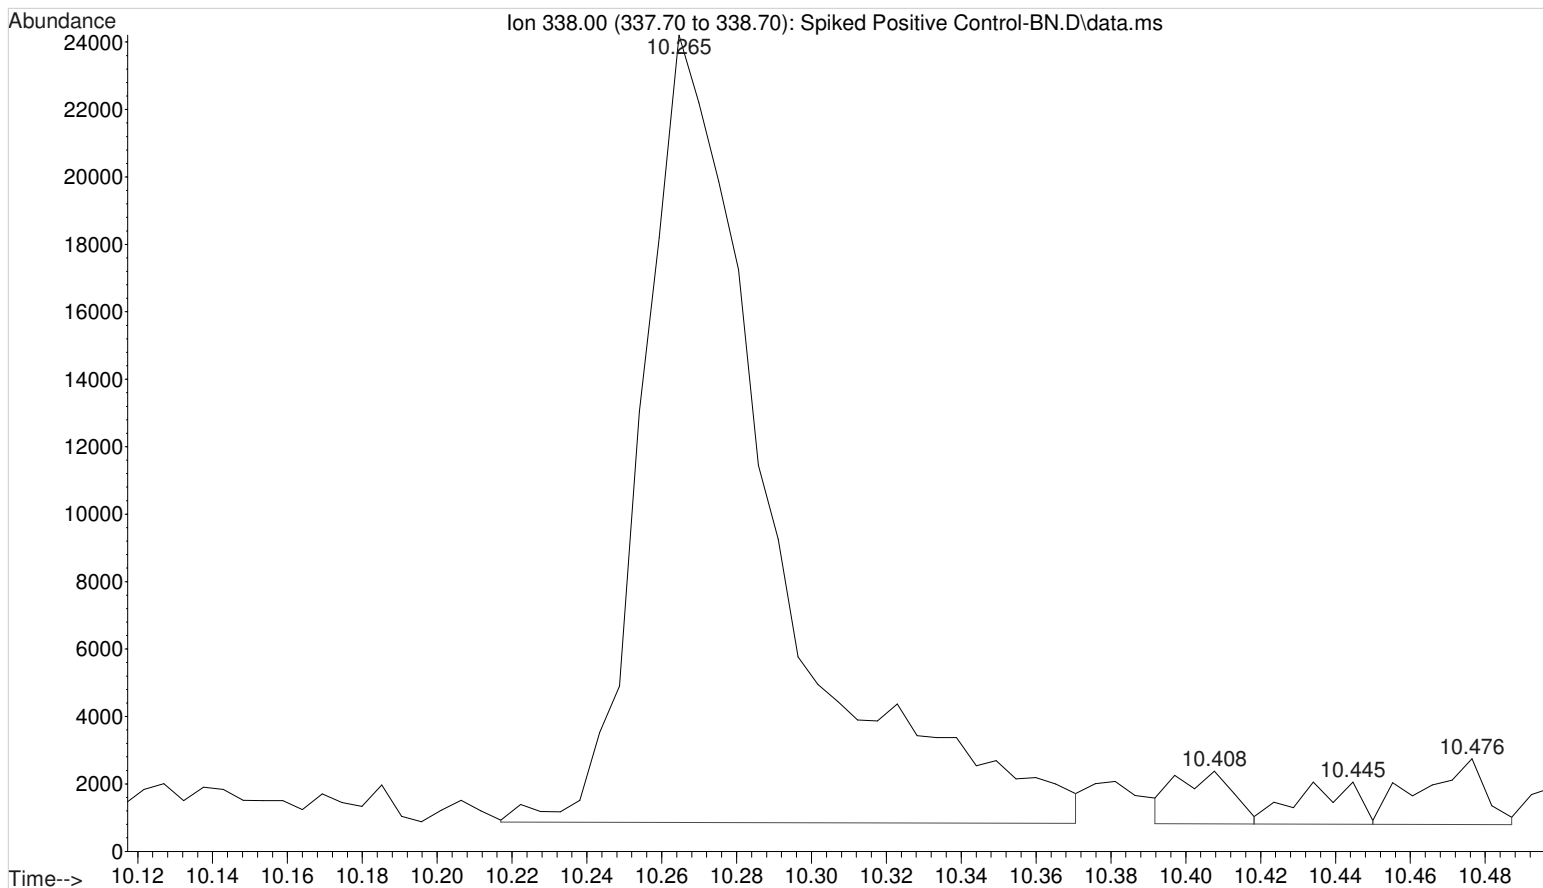



File : F:\10192016\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 19 Oct 2016 12:30 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name : Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

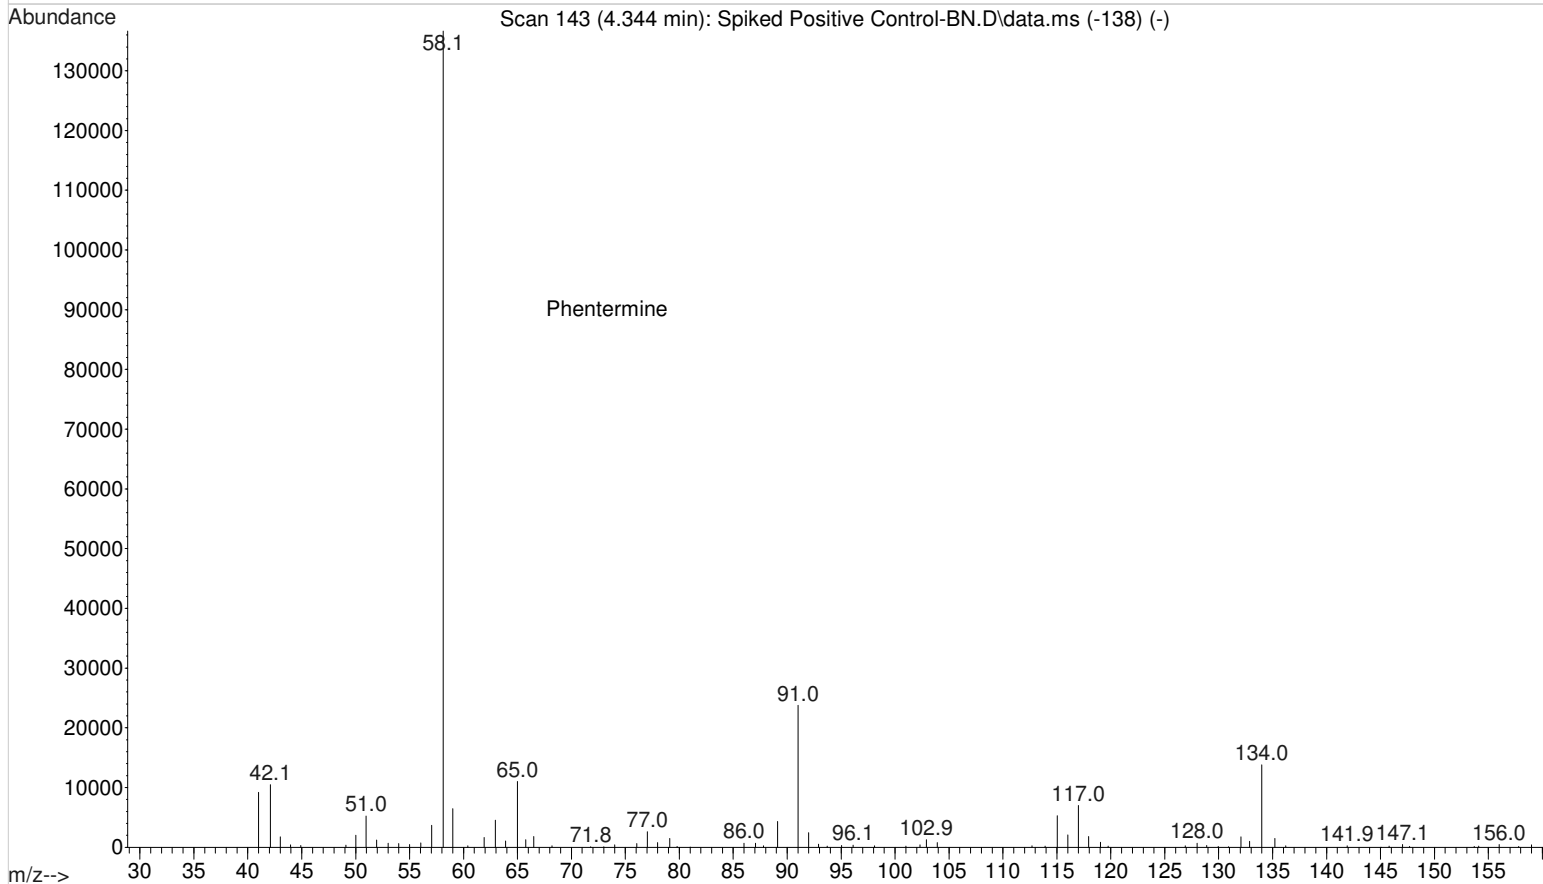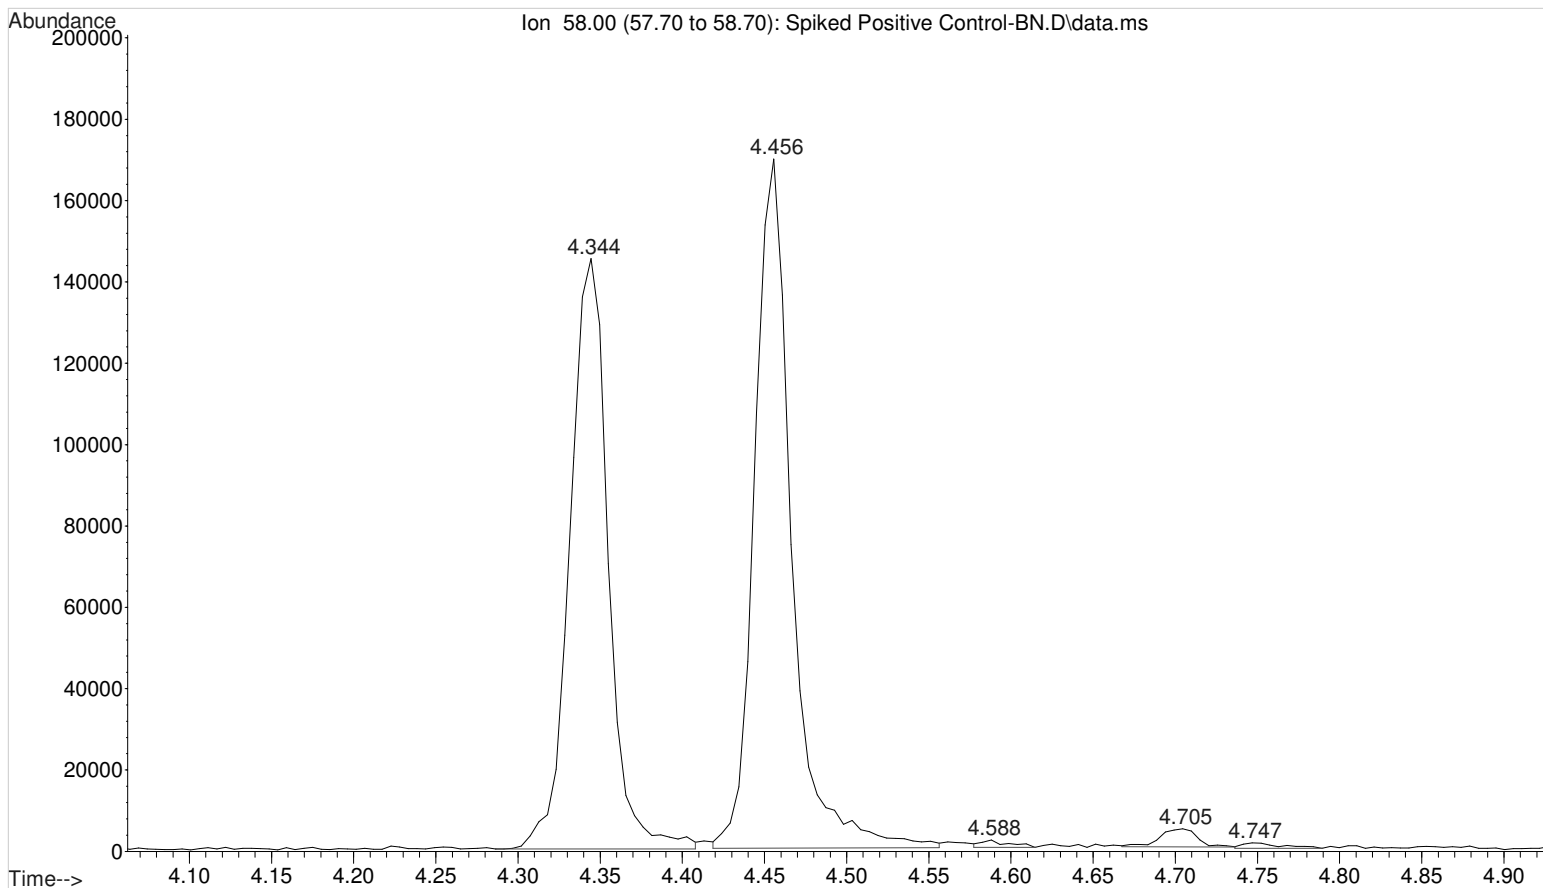



File : F:\10192016\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 19 Oct 2016 12:30 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name : Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

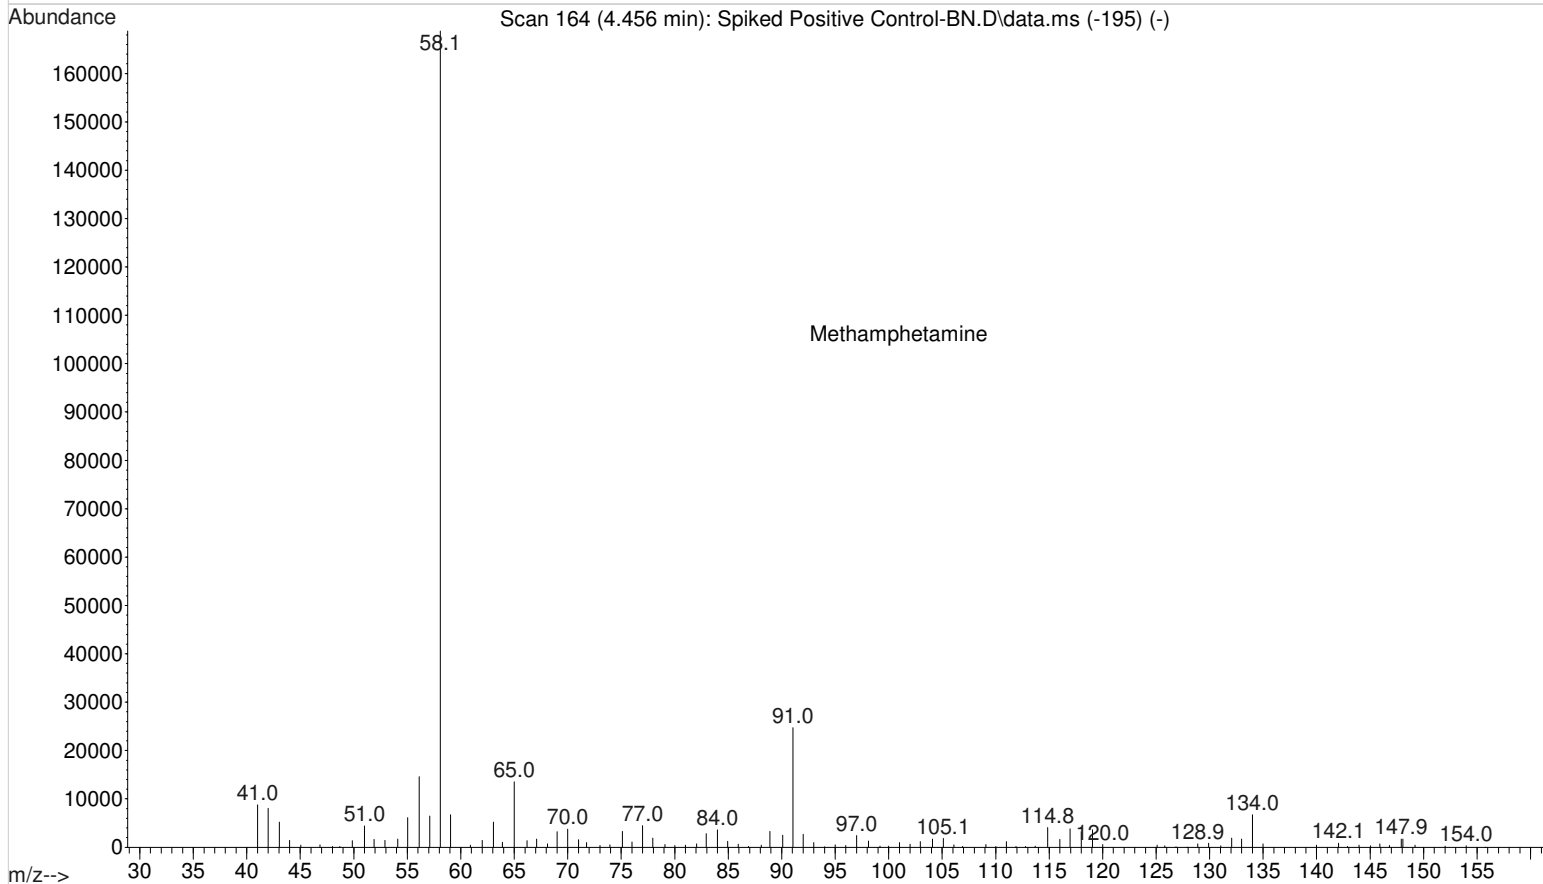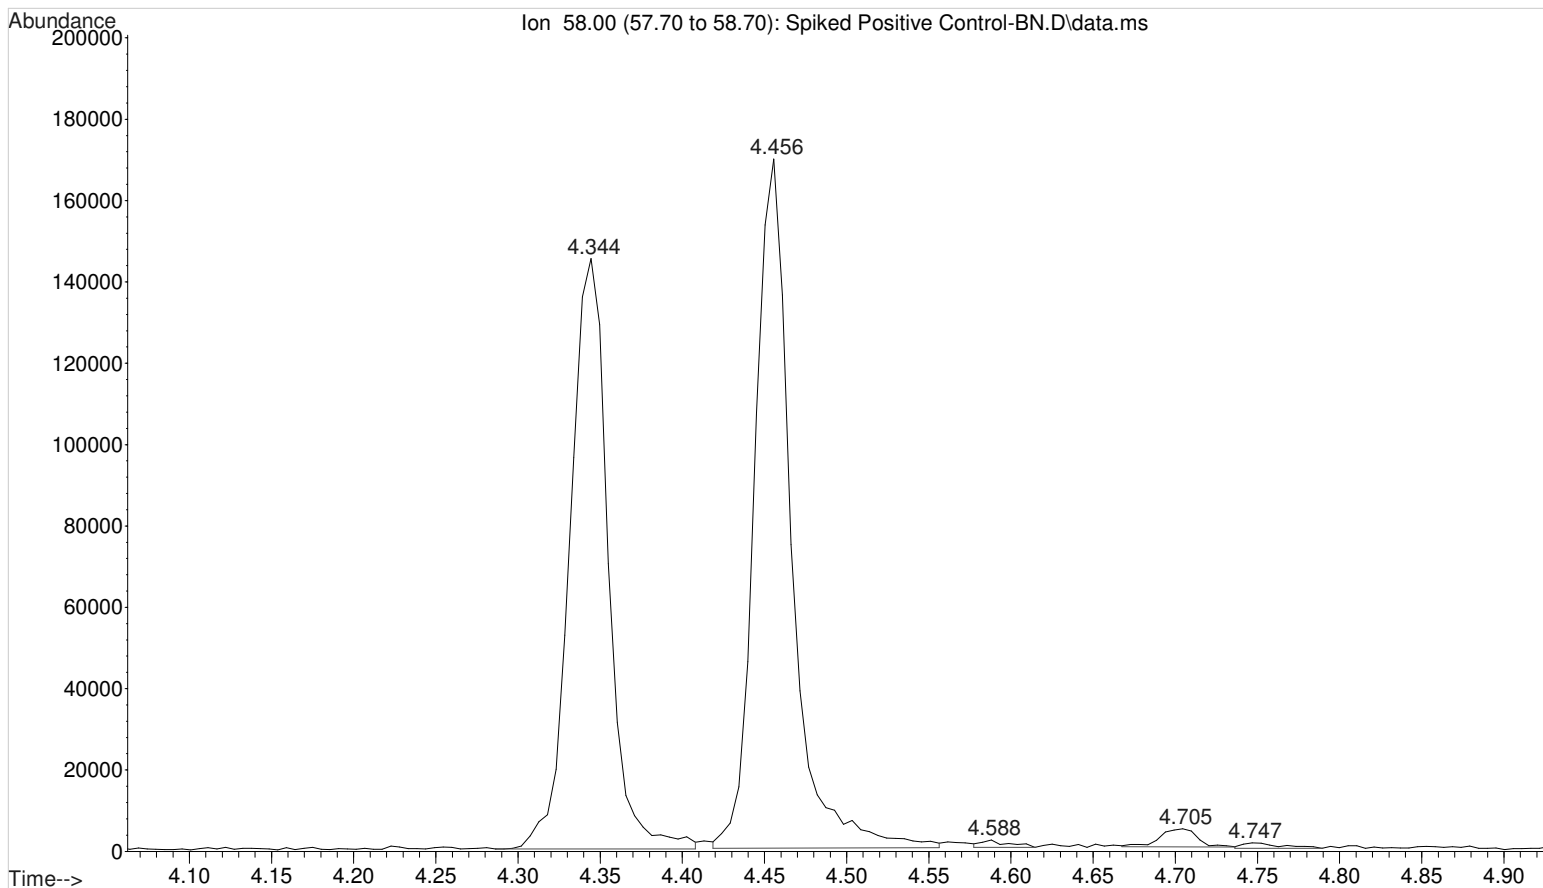



File : F:\10192016\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 19 Oct 2016 12:30 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

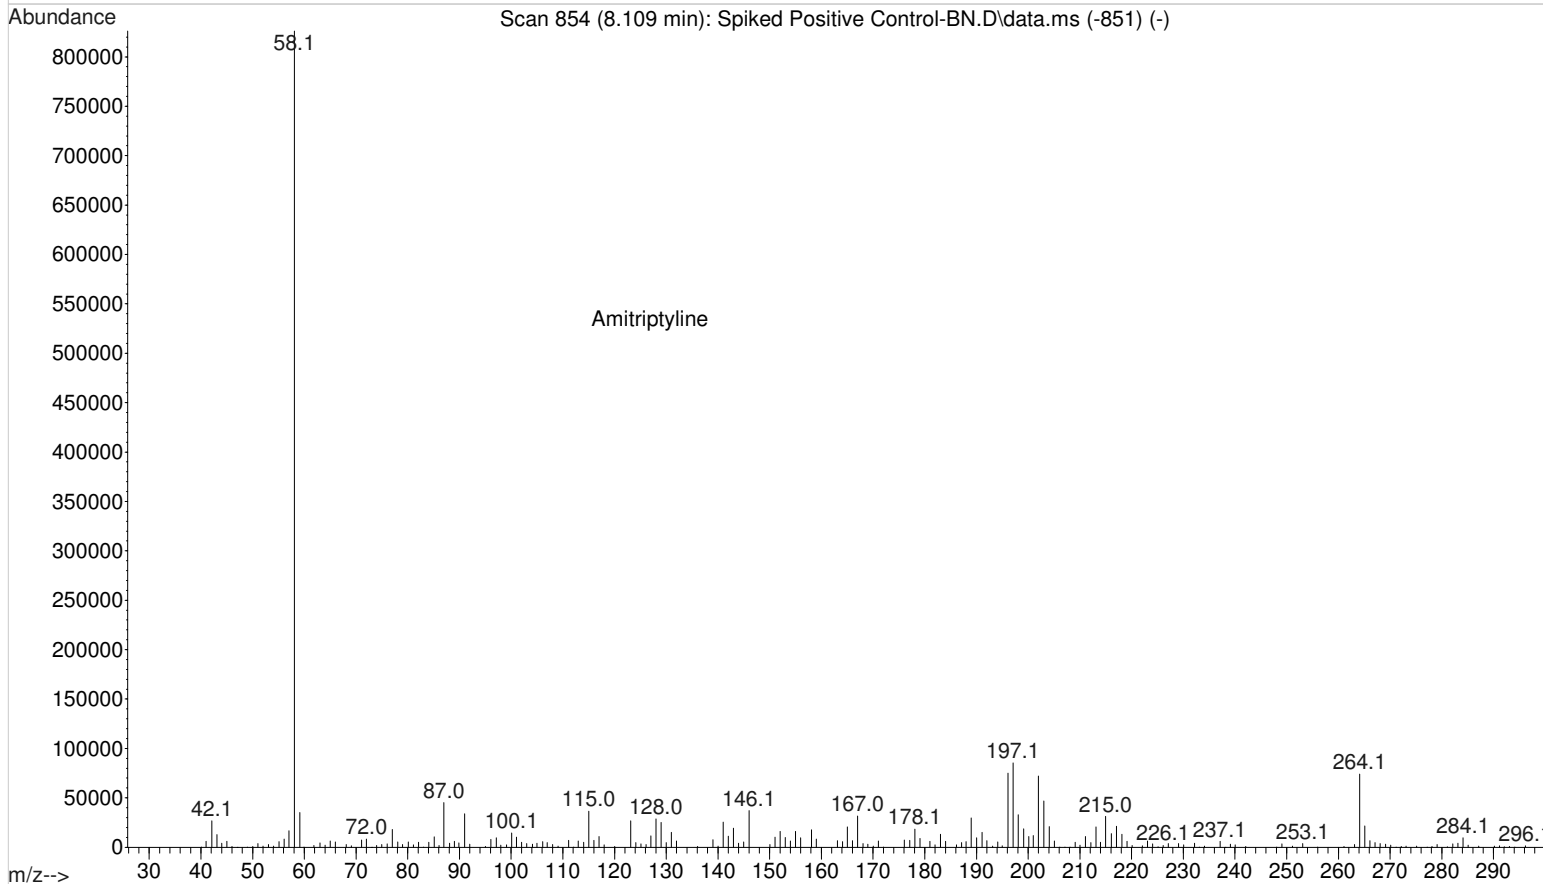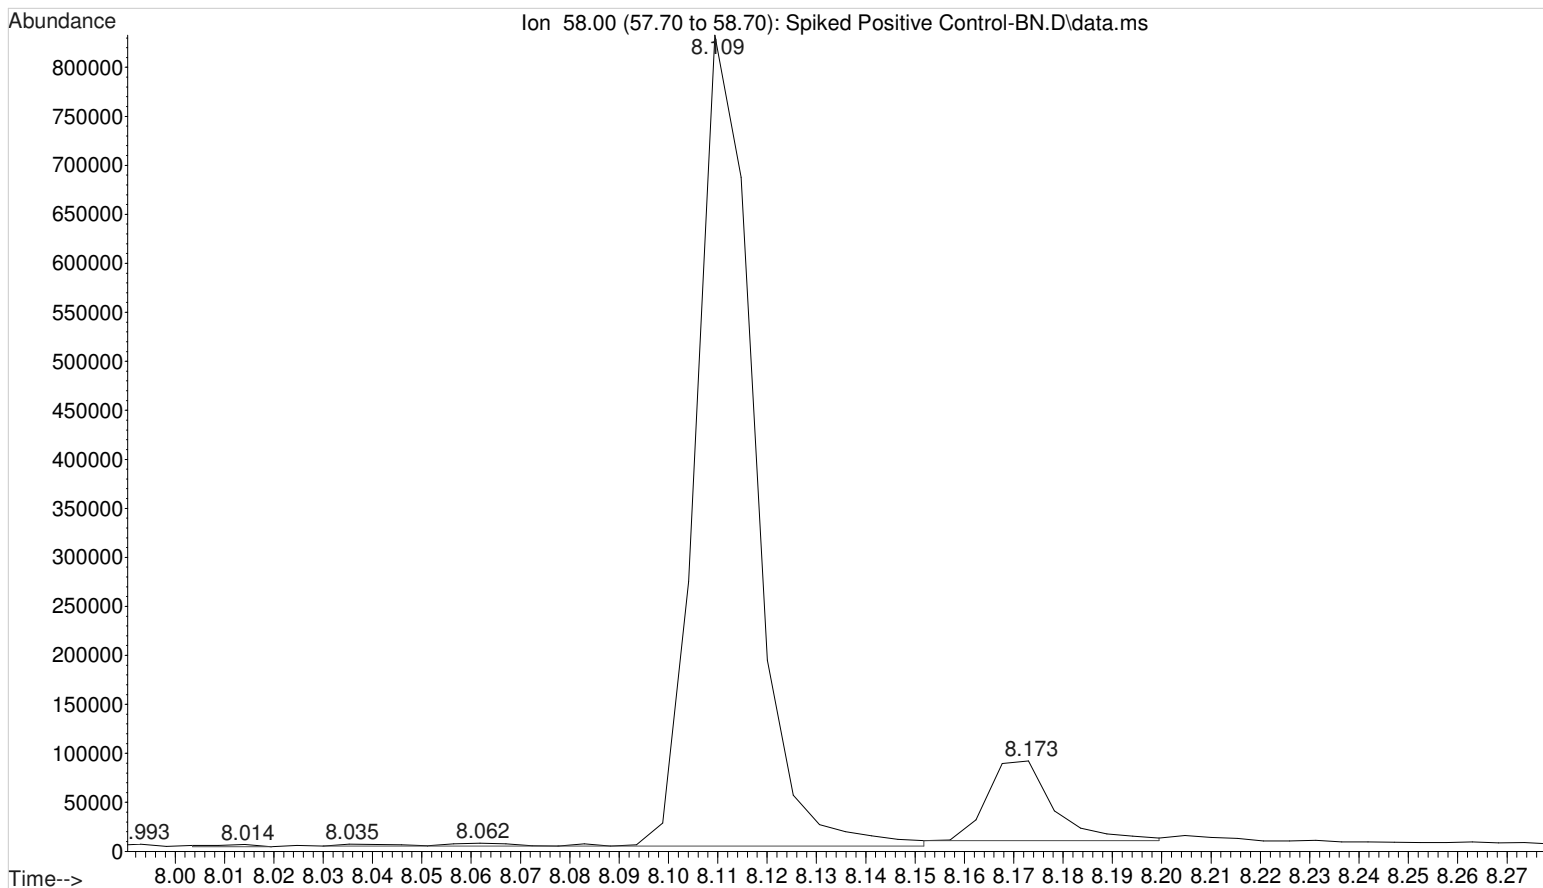

File : F:\10192016\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 19 Oct 2016 12:30 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

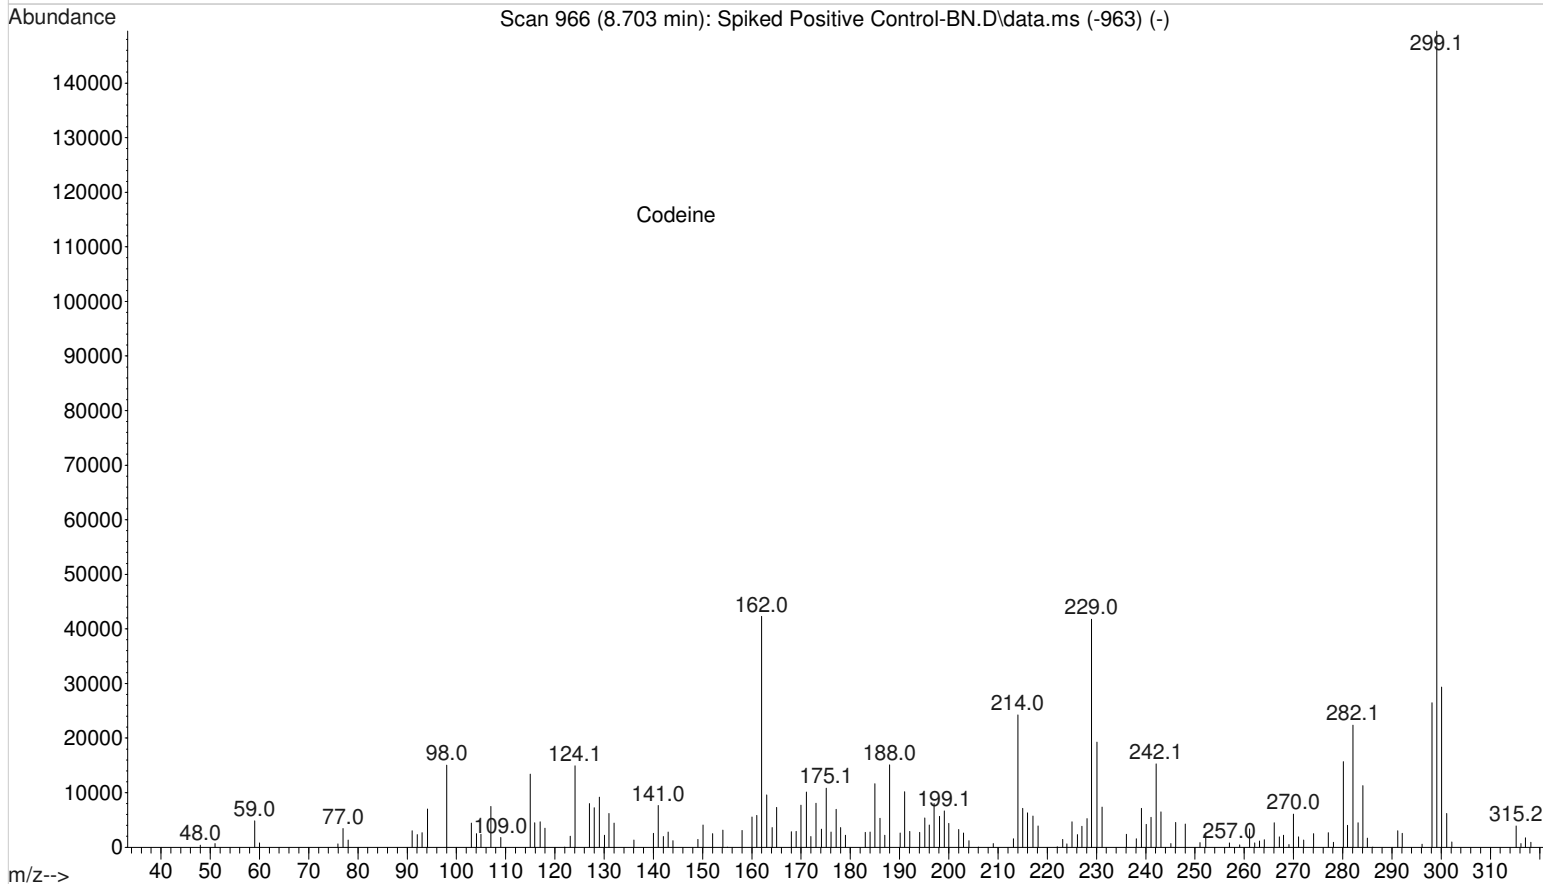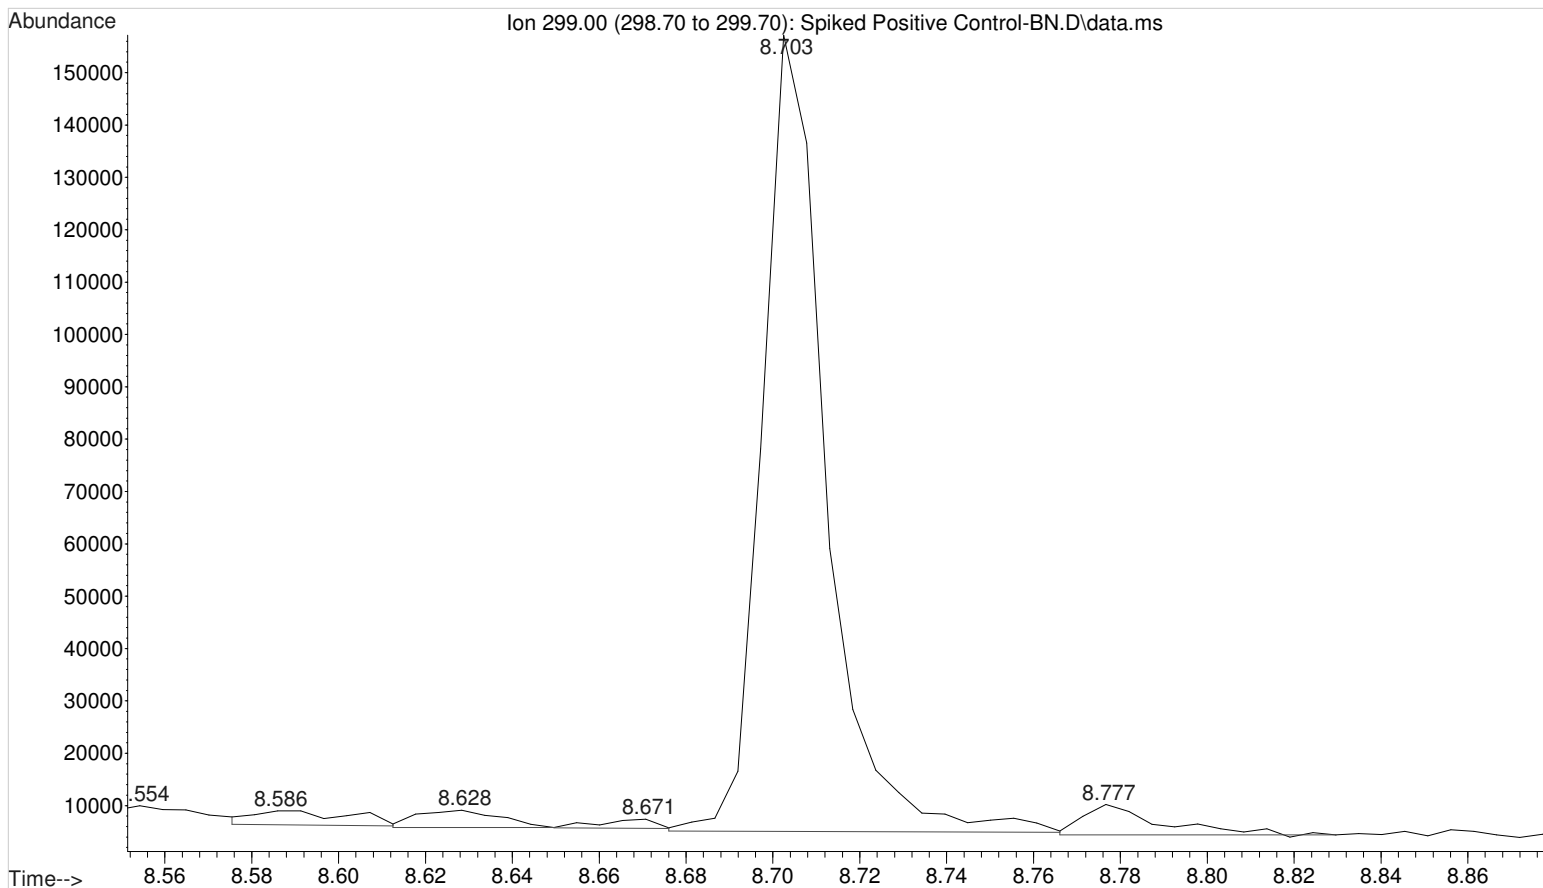


File : F:\10192016\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 19 Oct 2016 12:30 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

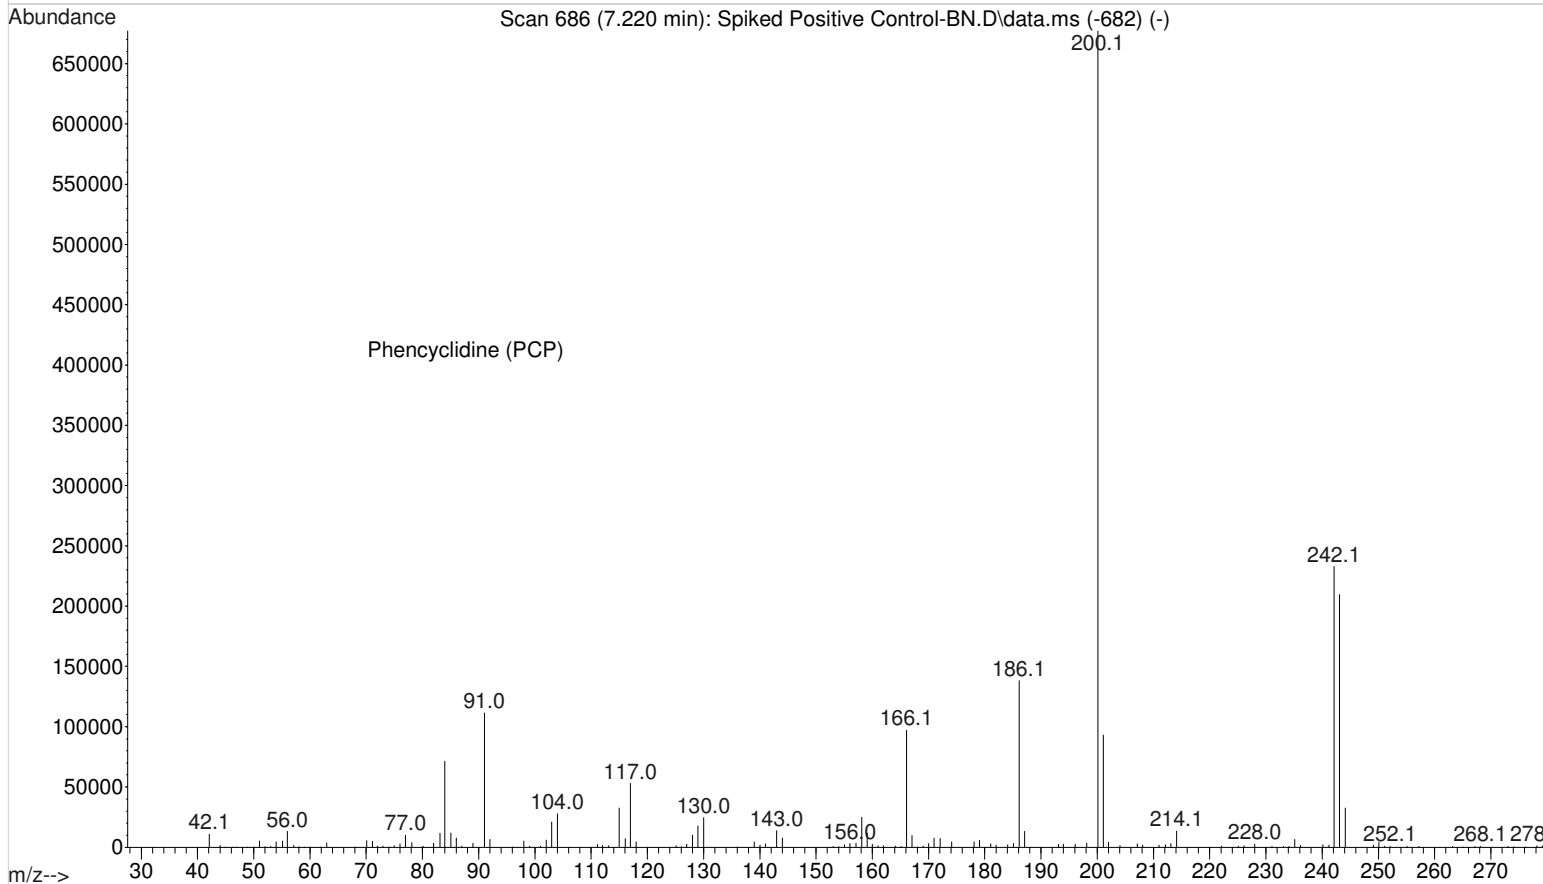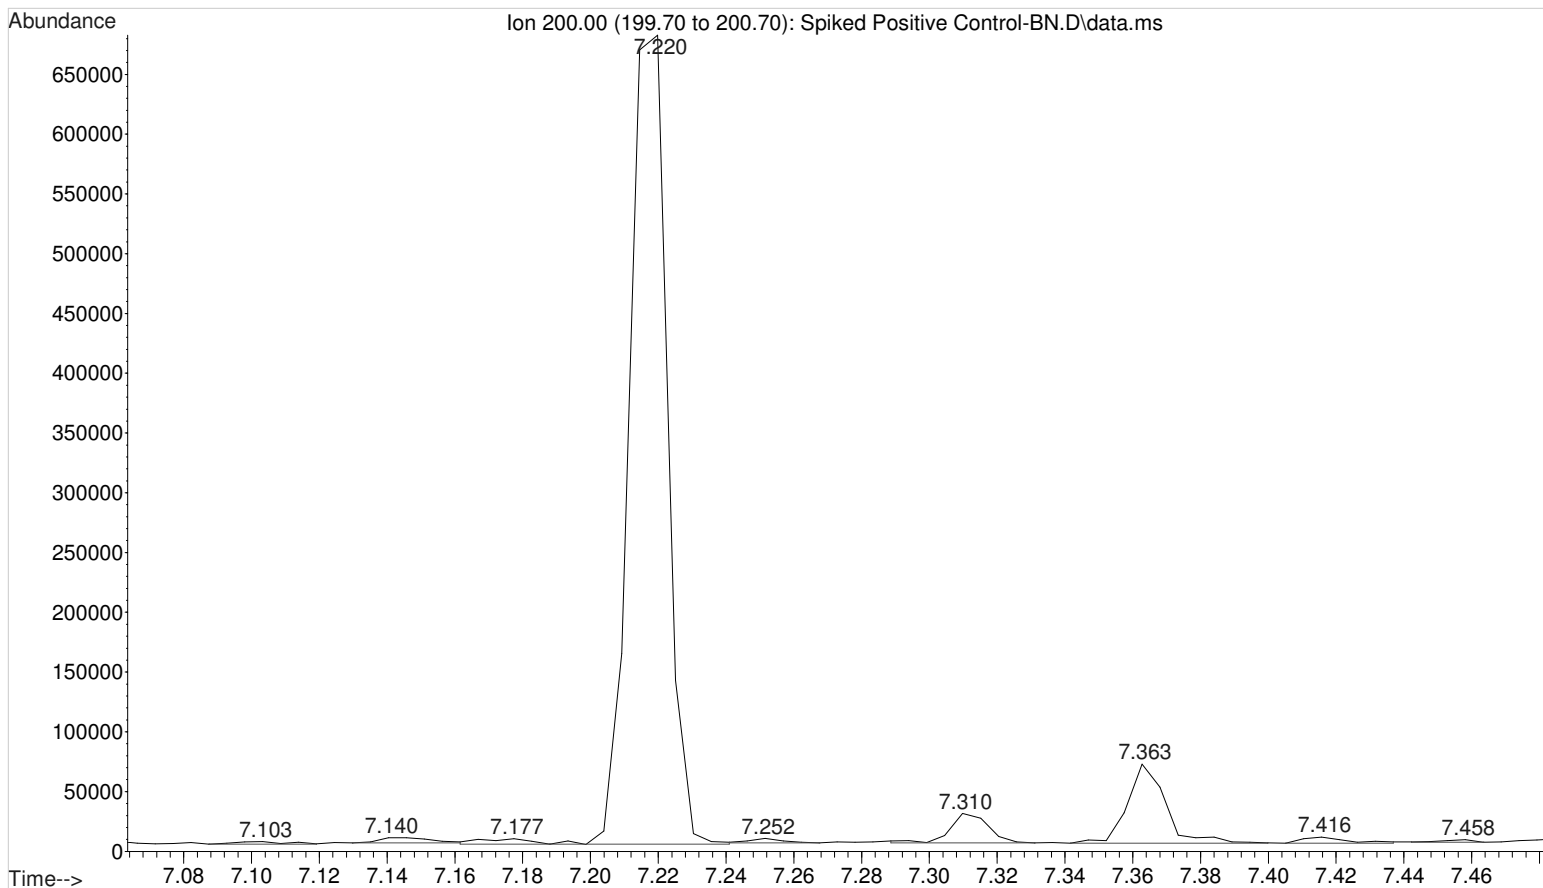


Handwritten signature

File :F:\10192016\Prerun Solvent Blankr.D
Operator : ISP\datastor
Acquired : 19 Oct 2016 13:16 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Pre-run Solvent Blank
Misc Info : Chloroform
Vial Number: 100

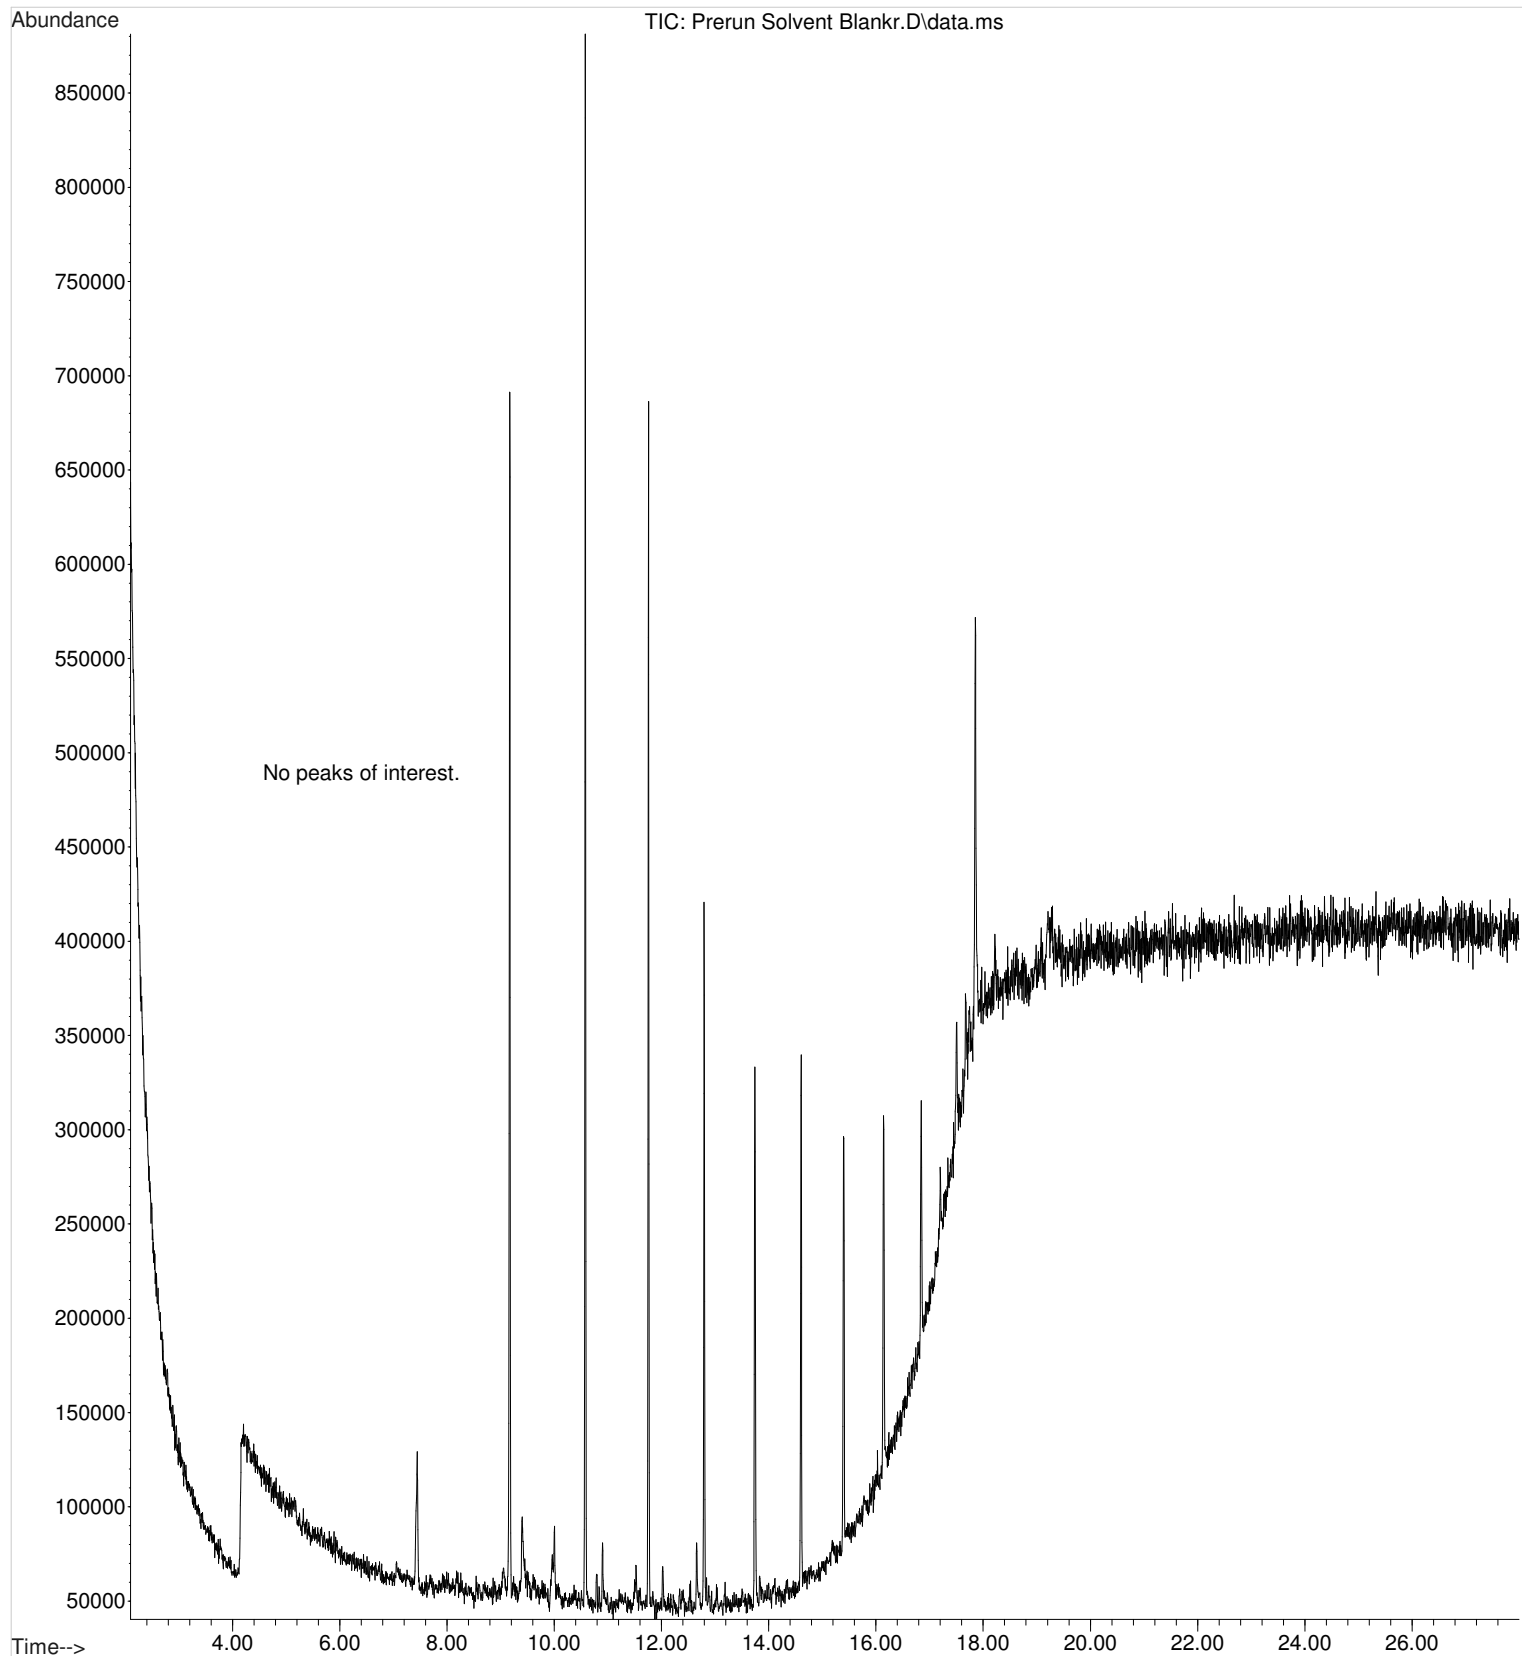


Handwritten signature

File :F:\10192016\prbLK2r.D
Operator : ISP\datastor
Acquired : 19 Oct 2016 14:57 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Solvent Blank
Misc Info : Chloroform
Vial Number: 99


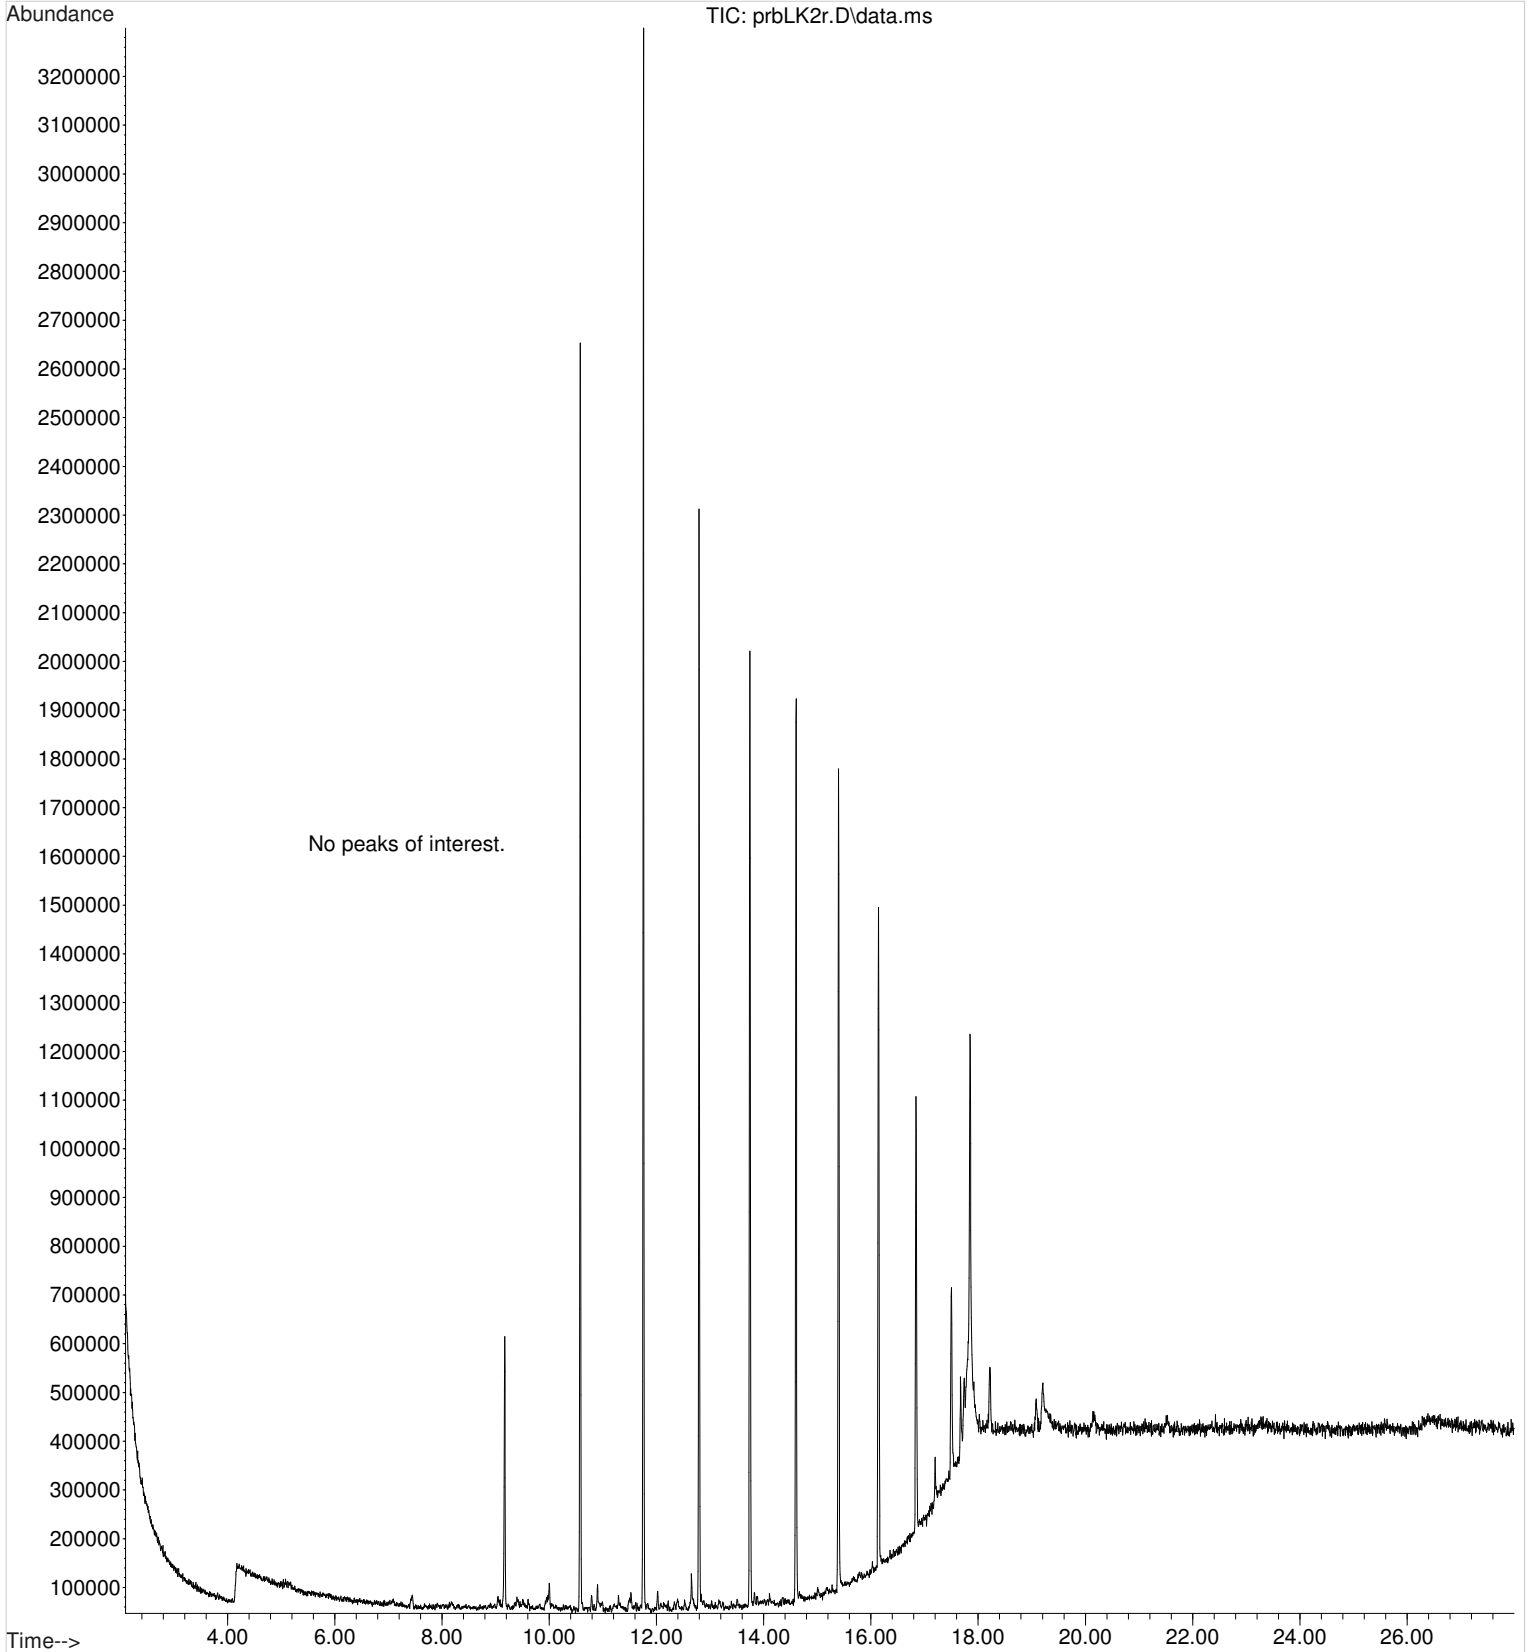


Handwritten signature



File : F:\10192016\Negative Control-BNr.D
Operator : ISP\datastor
Acquired : 19 Oct 2016 13:49 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B1013
Misc Info : Analytical Method 3.6.1
Vial Number: 1

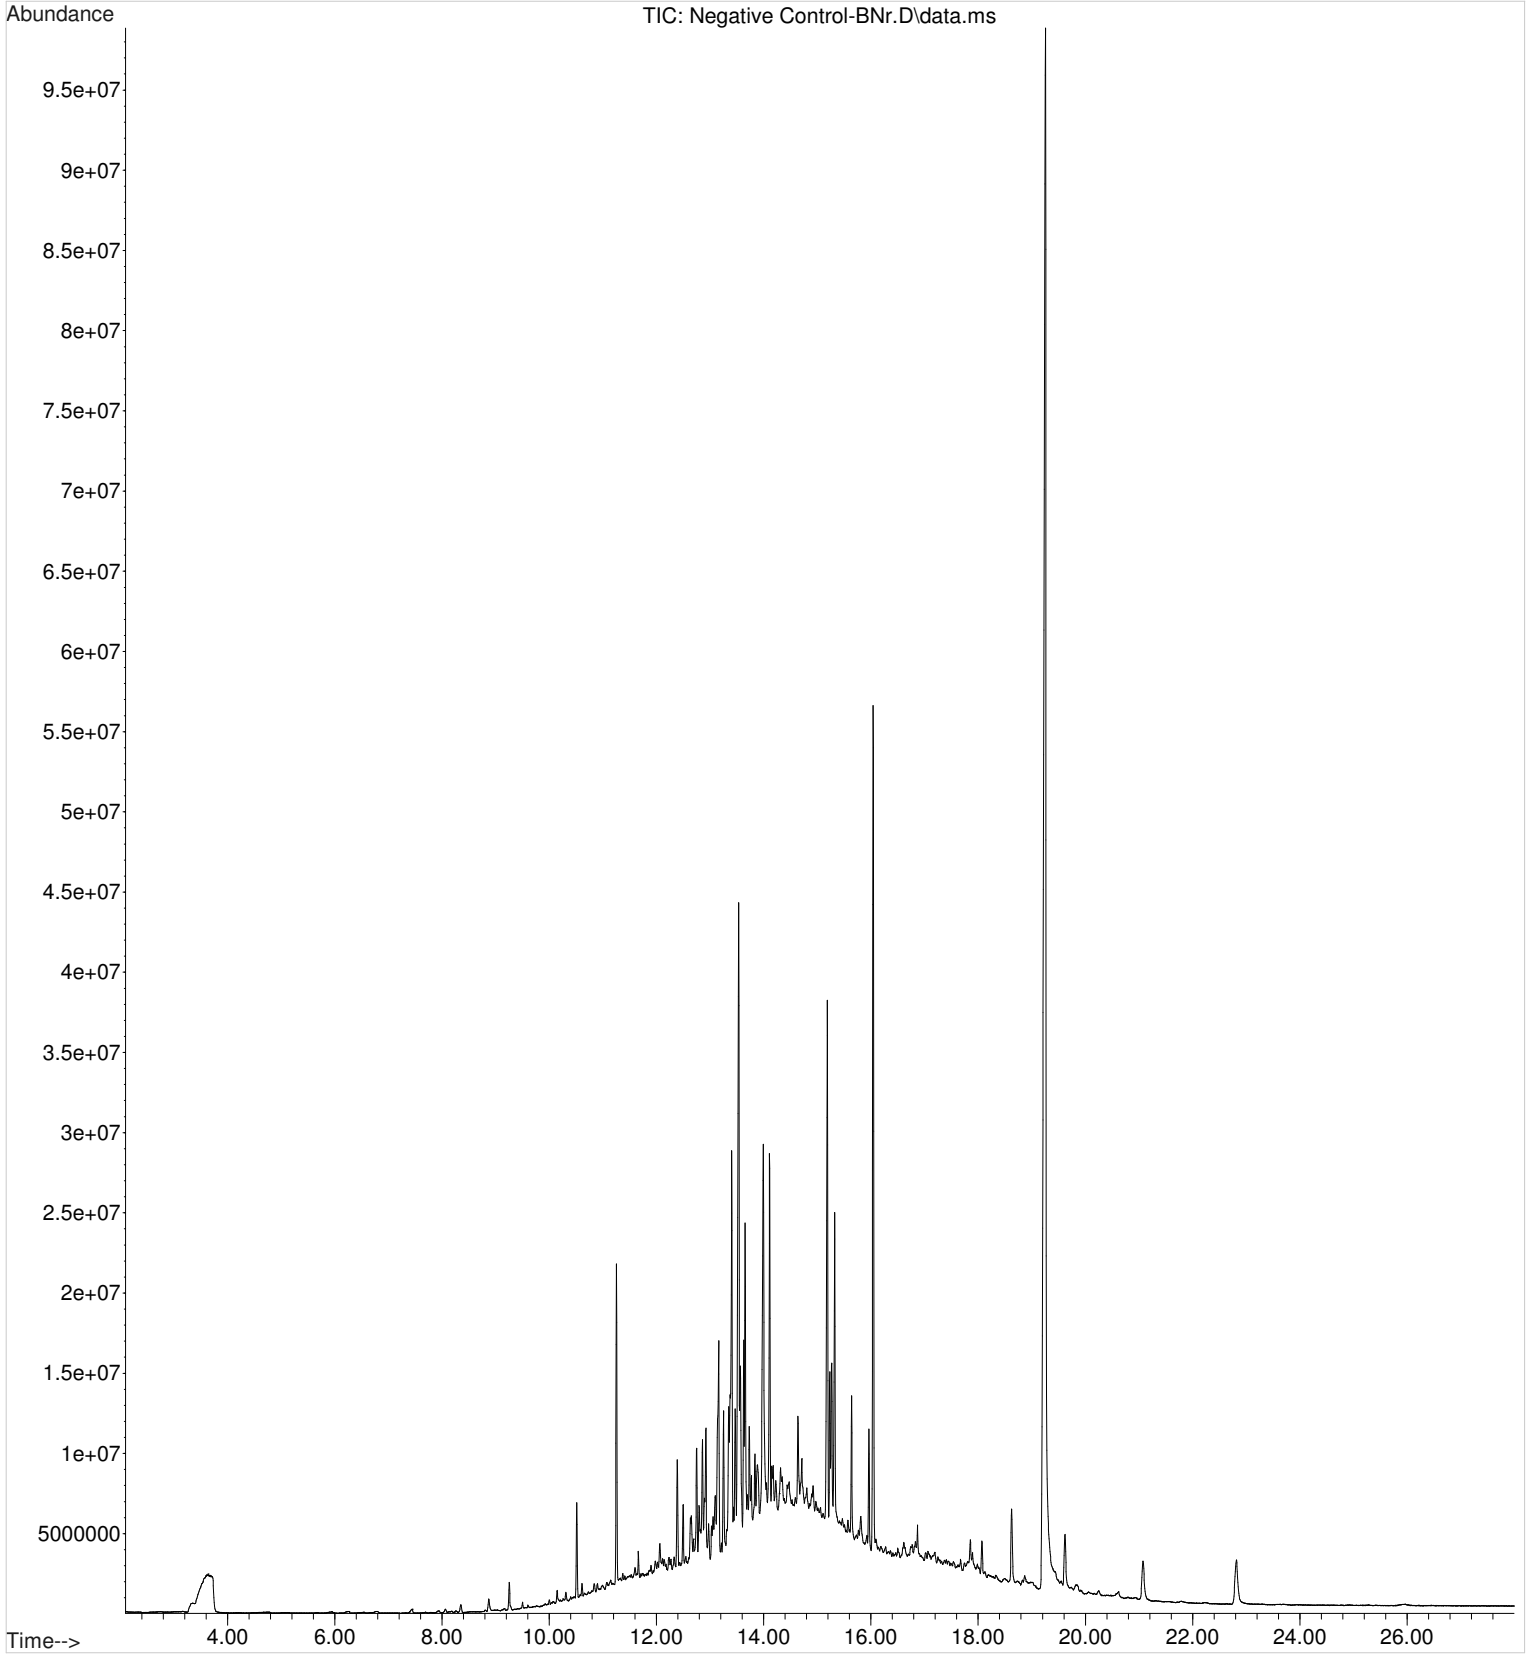


File : F:\10192016\Negative Control-BNr.D
Operator : ISP\datastor
Acquired : 19 Oct 2016 13:49 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name : Negative Control - Utak Lot B1013
Misc Info : Analytical Method 3.6.1
Vial Number: 1

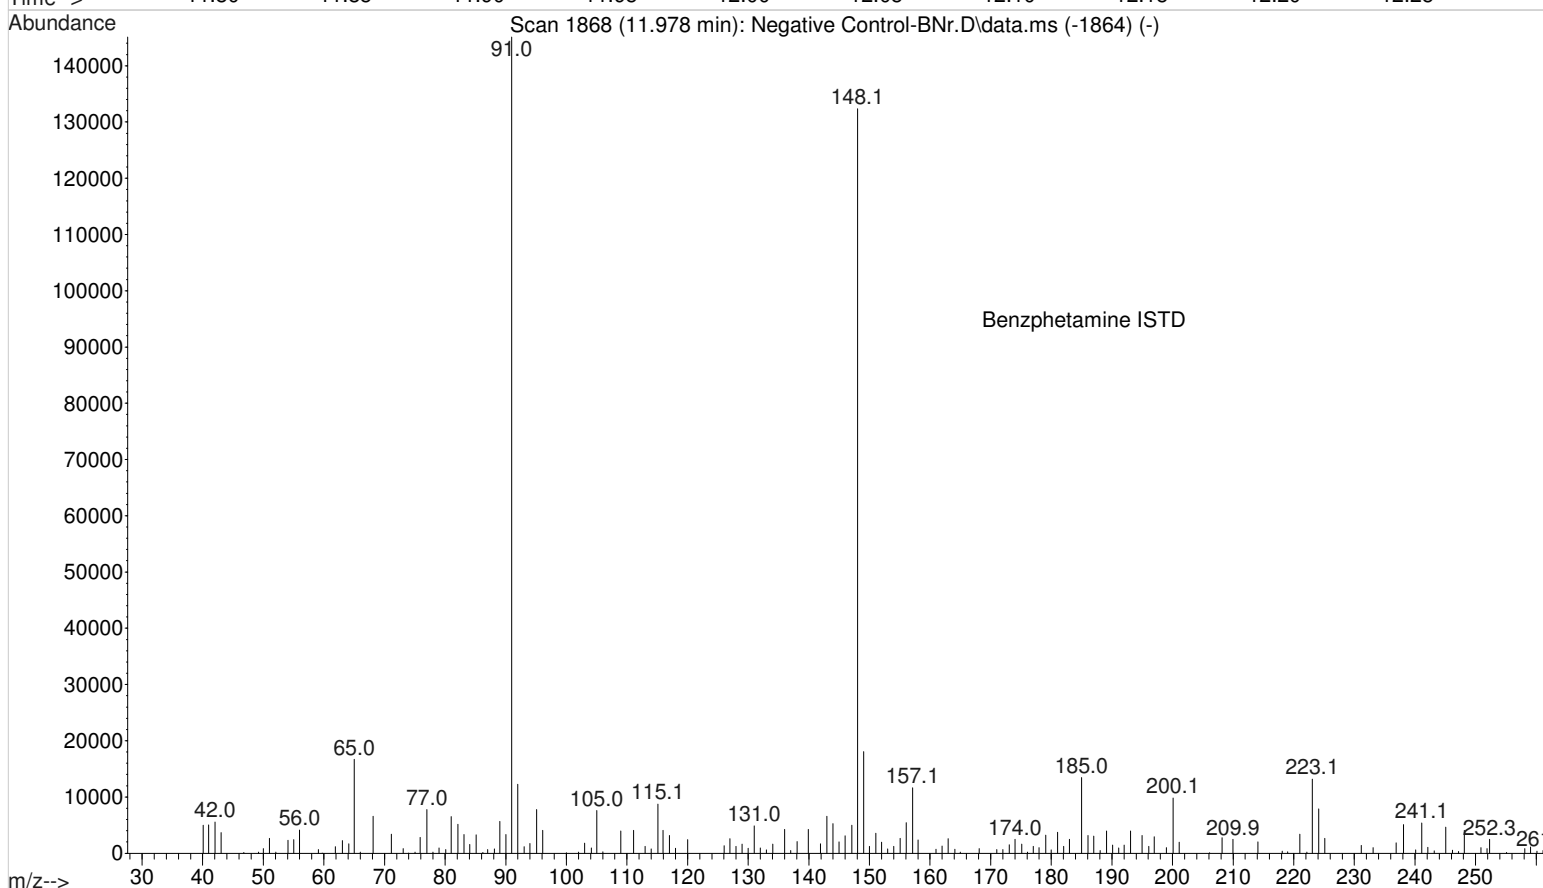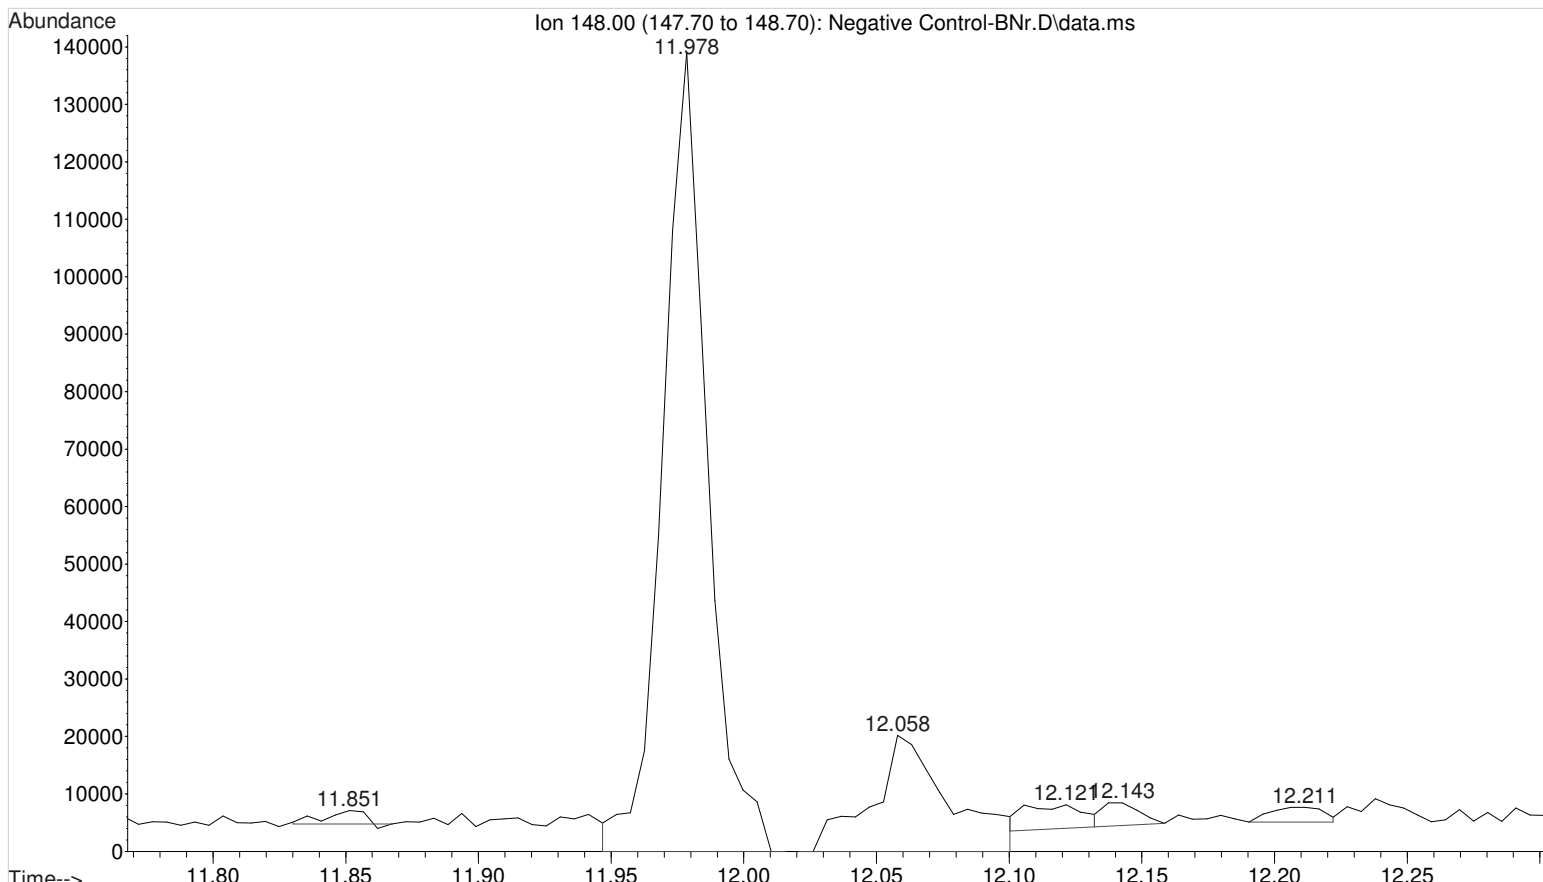



File : F:\10192016\Negative Control-BNr.D
Operator : ISP\datastor
Acquired : 19 Oct 2016 13:49 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name : Negative Control - Utak Lot B1013
Misc Info : Analytical Method 3.6.1
Vial Number: 1

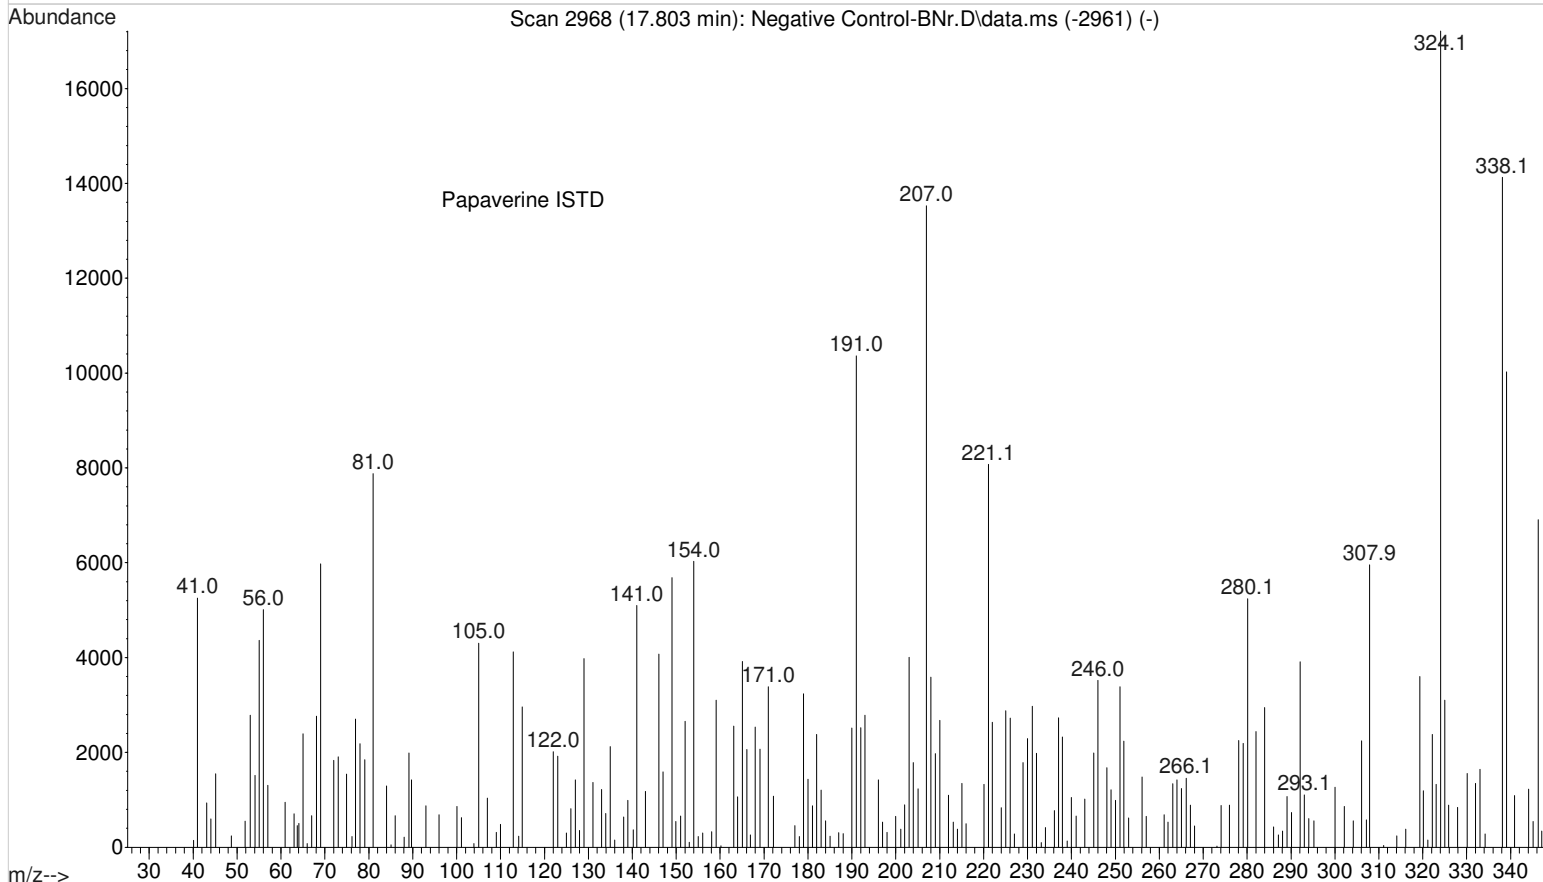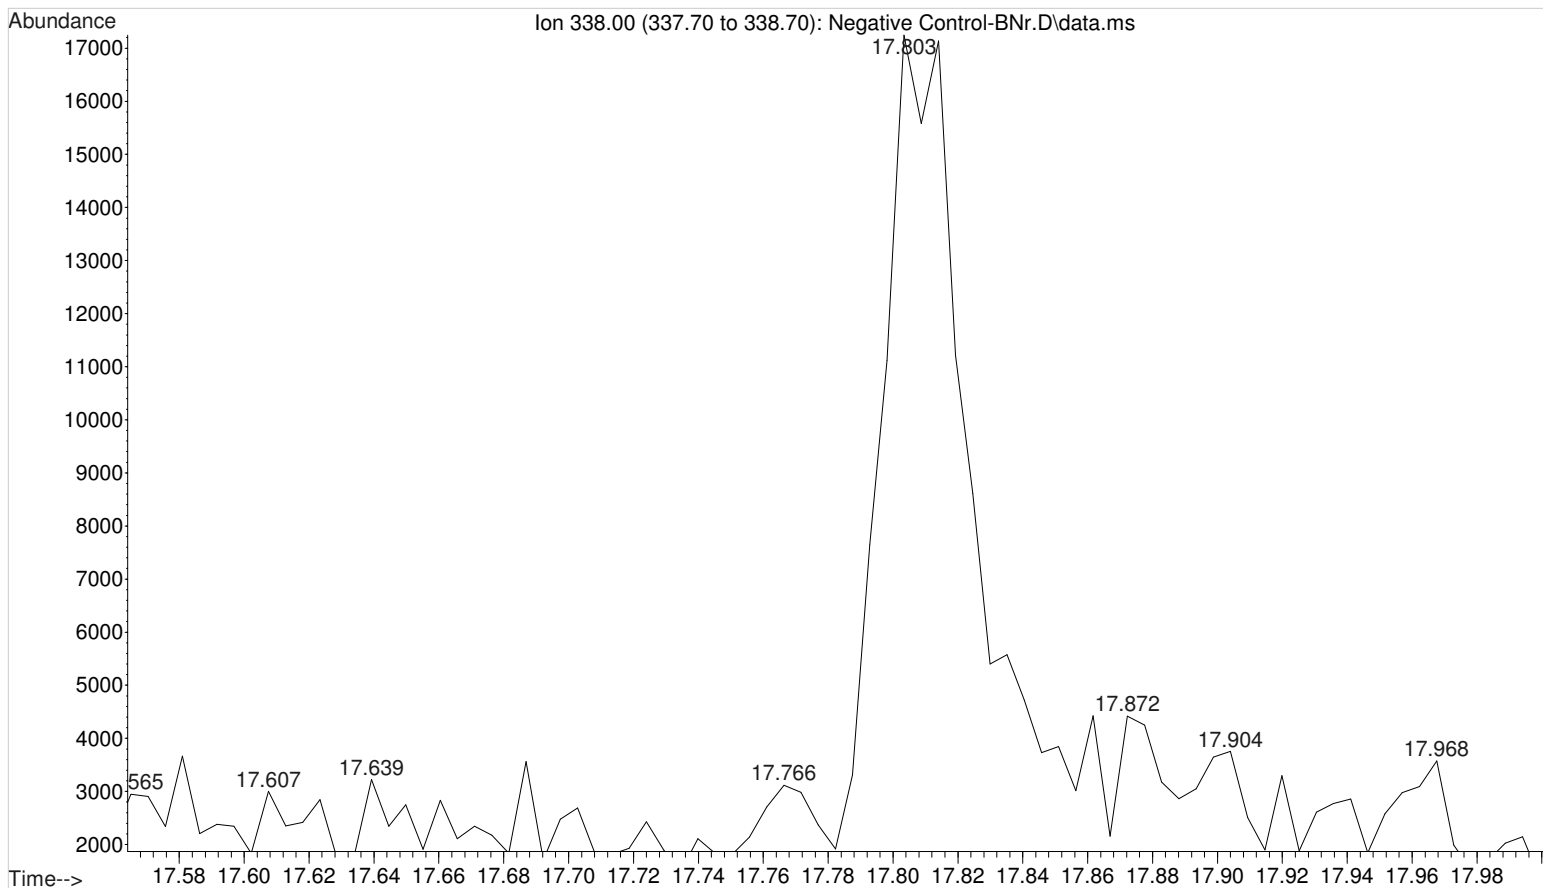



File :F:\10192016\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 19 Oct 2016 14:23 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

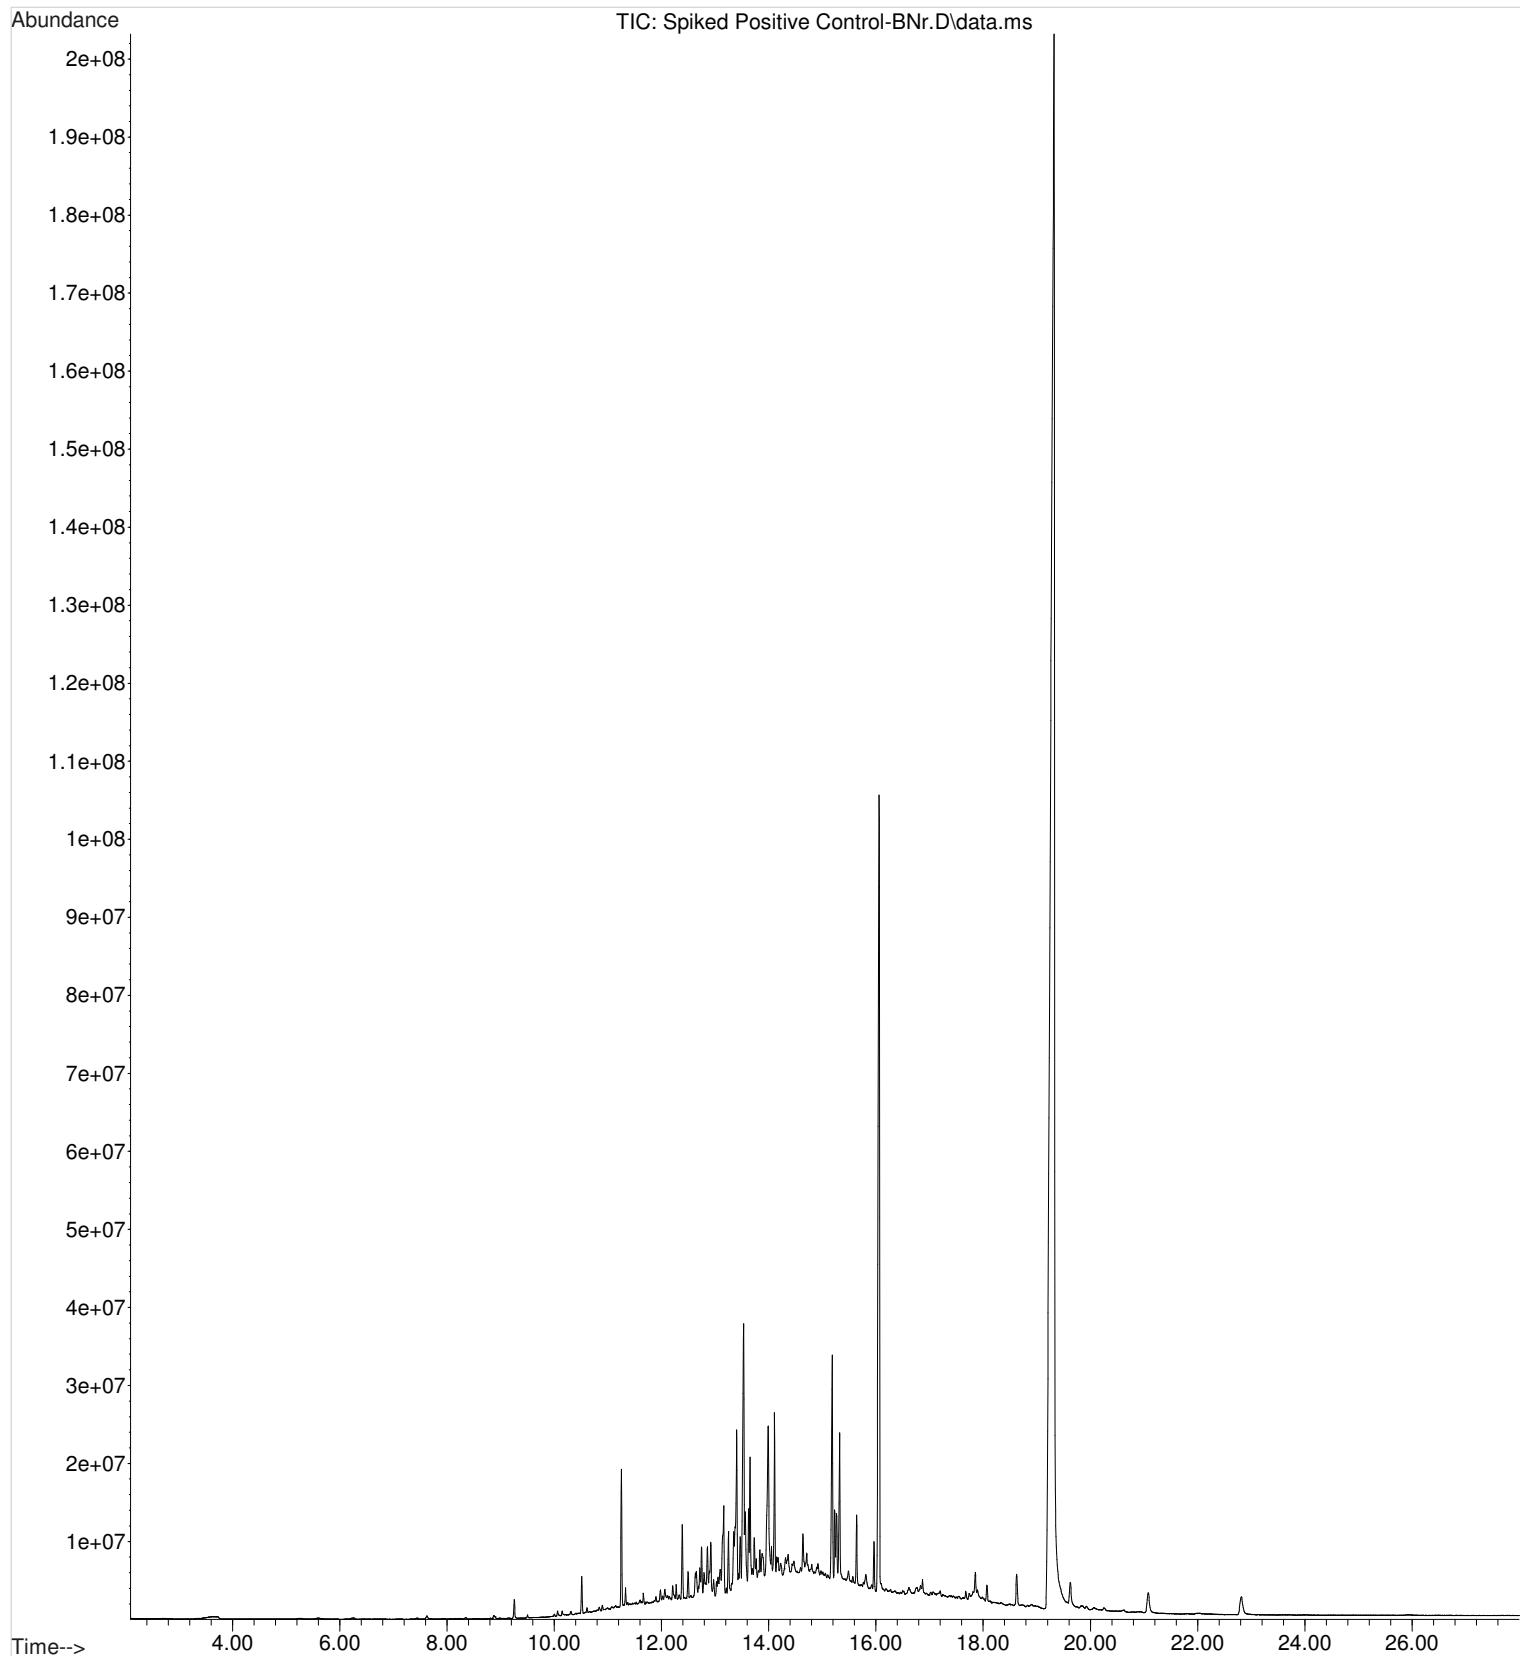



File : F:\10192016\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 19 Oct 2016 14:23 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

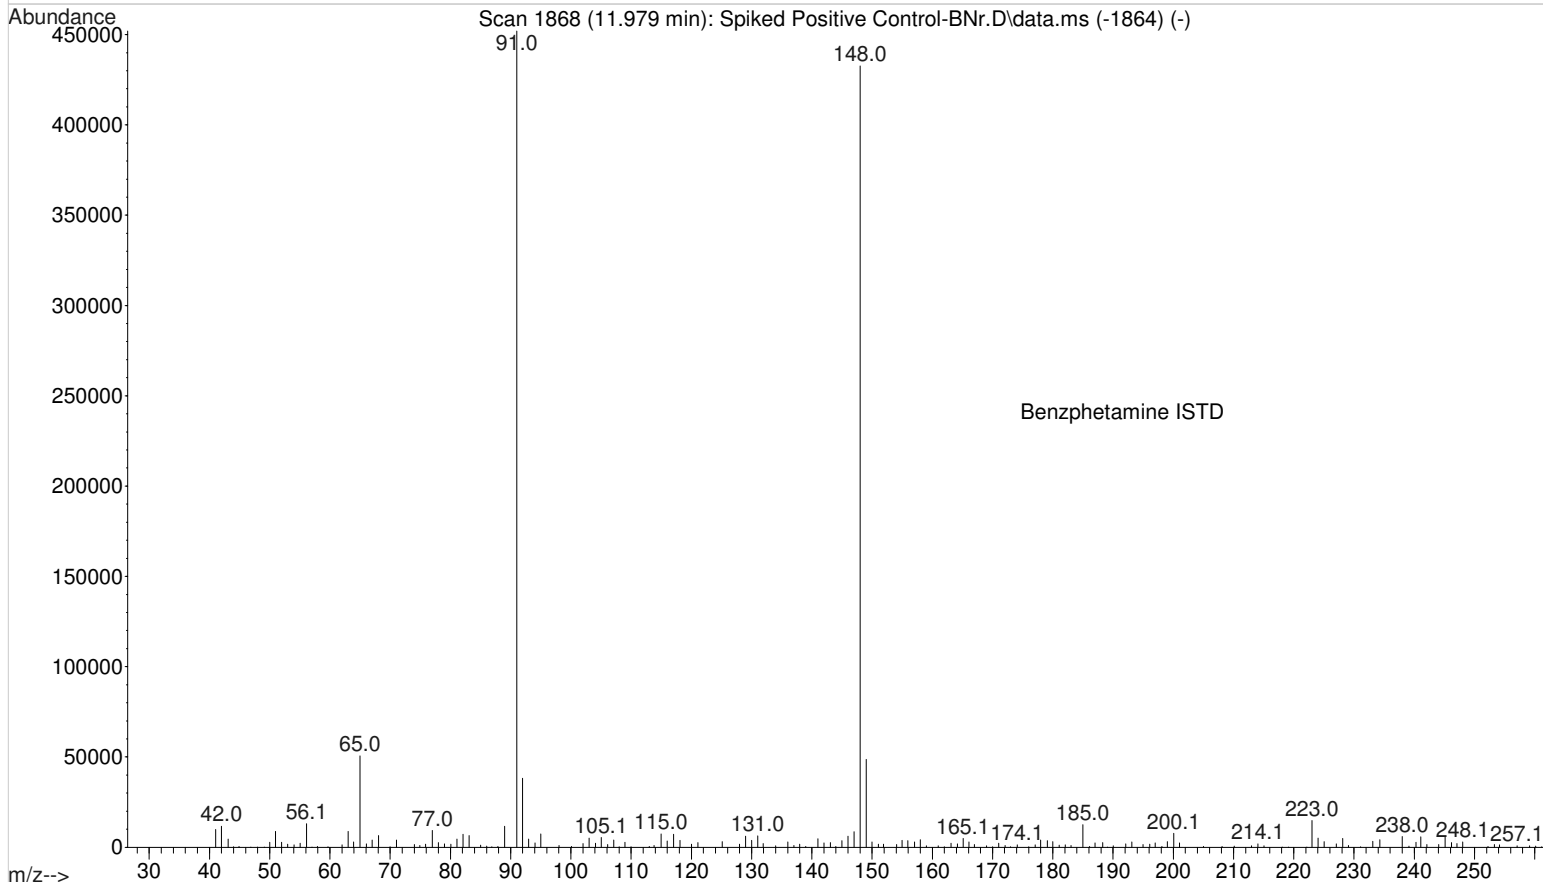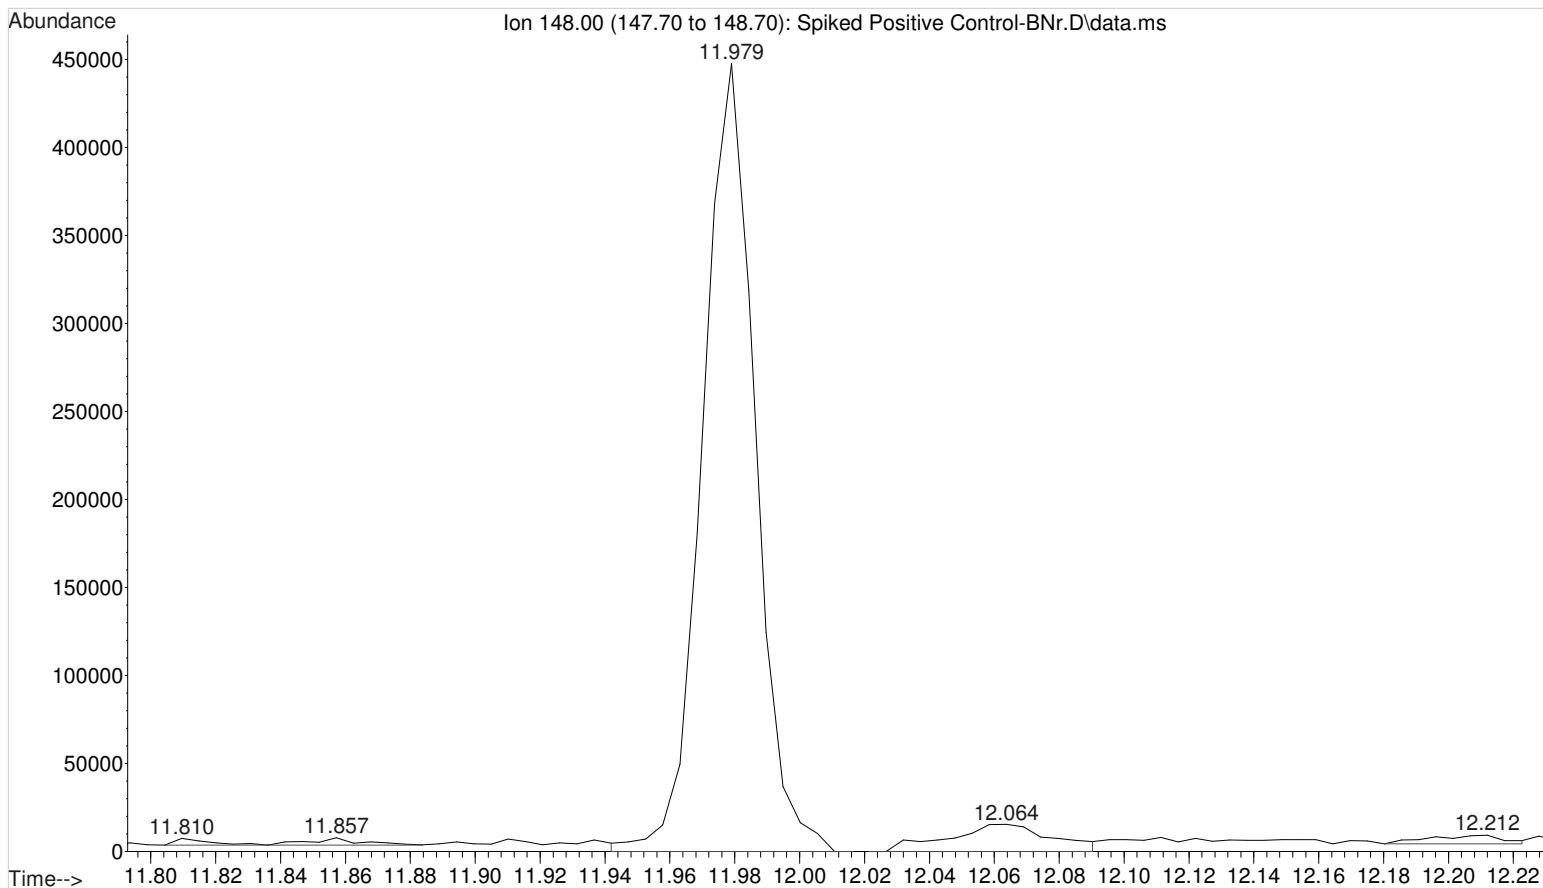



File : F:\10192016\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 19 Oct 2016 14:23 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

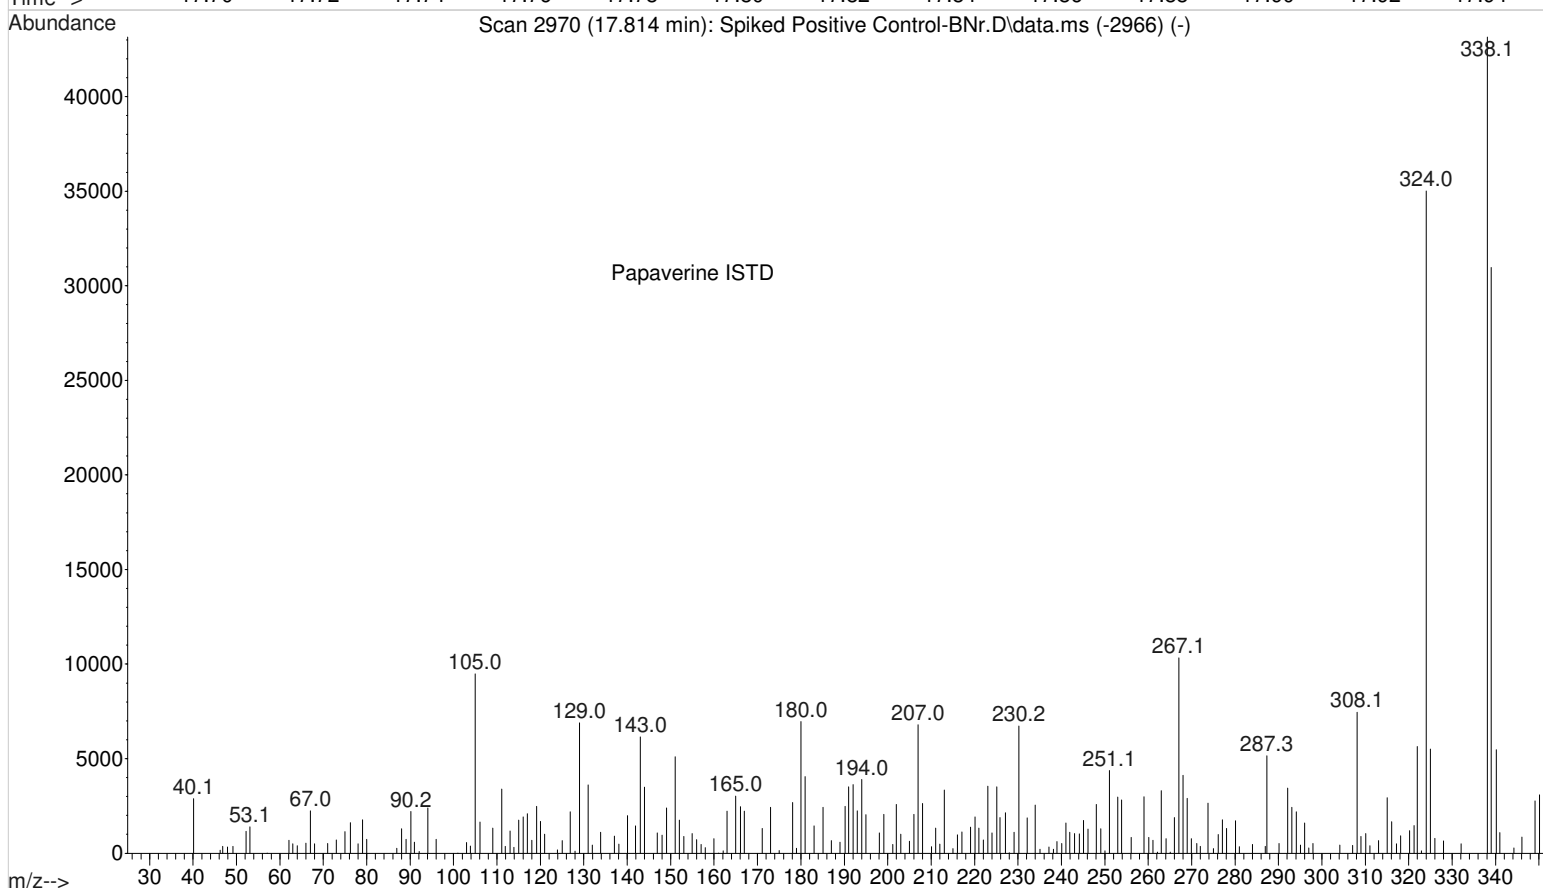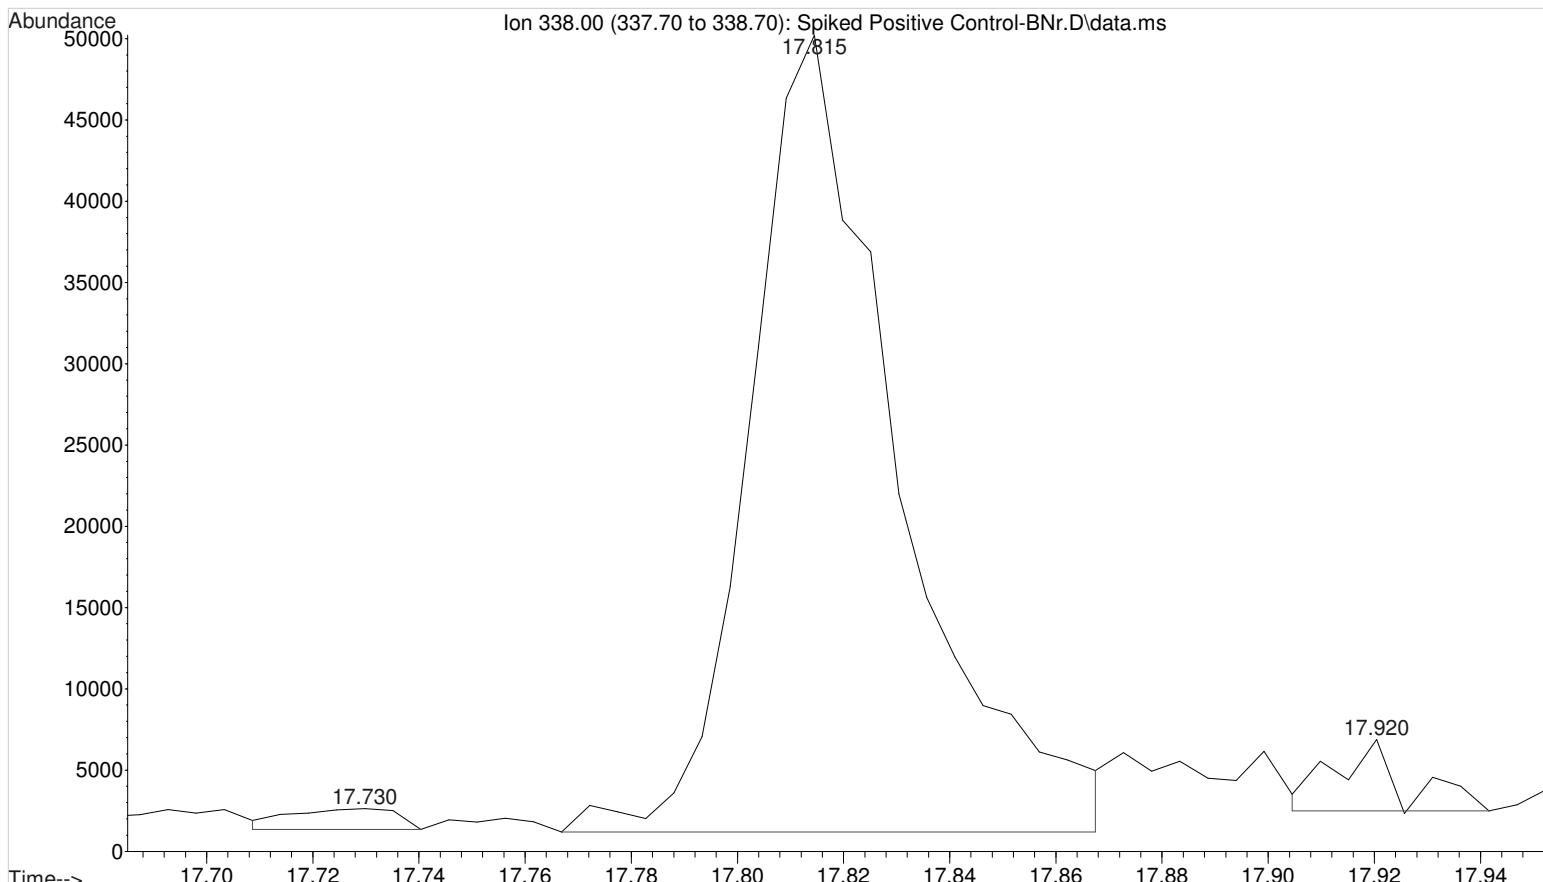



File : F:\10192016\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 19 Oct 2016 14:23 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

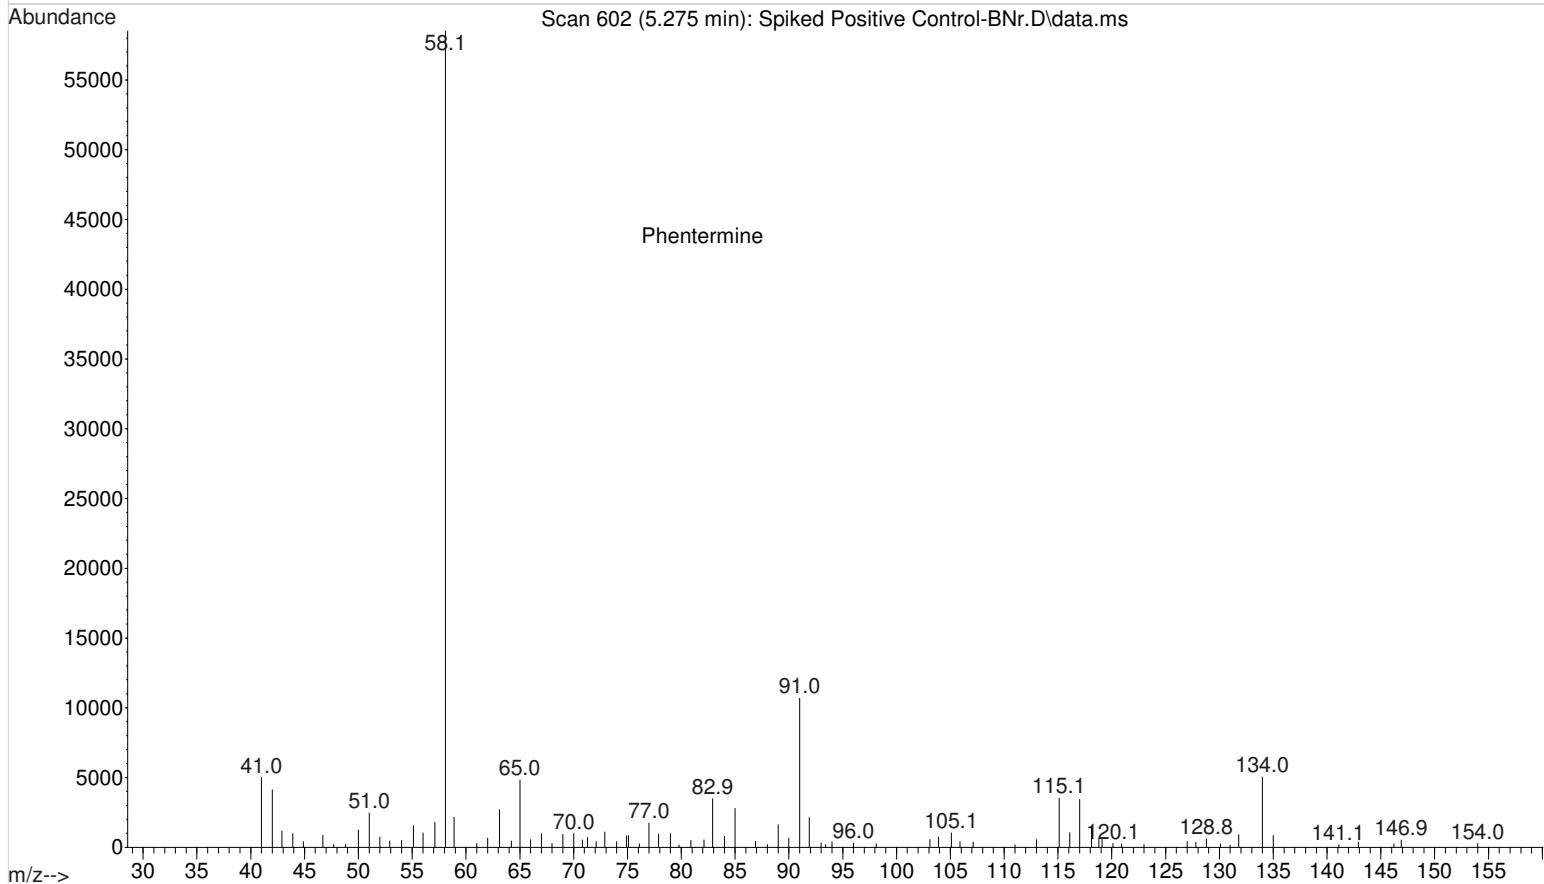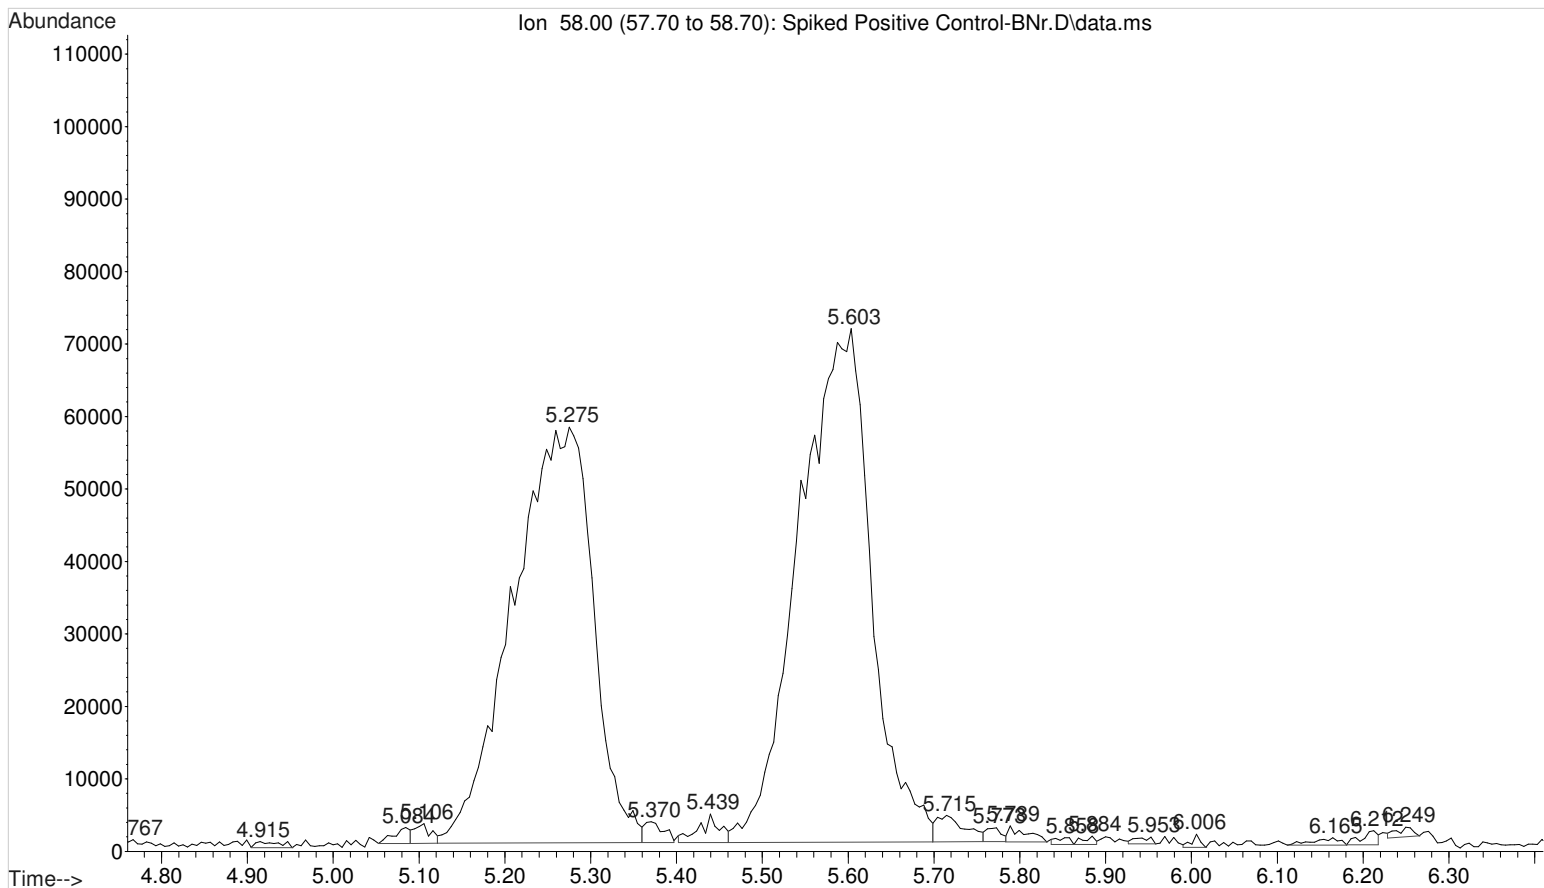



File : F:\10192016\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 19 Oct 2016 14:23 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name : Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

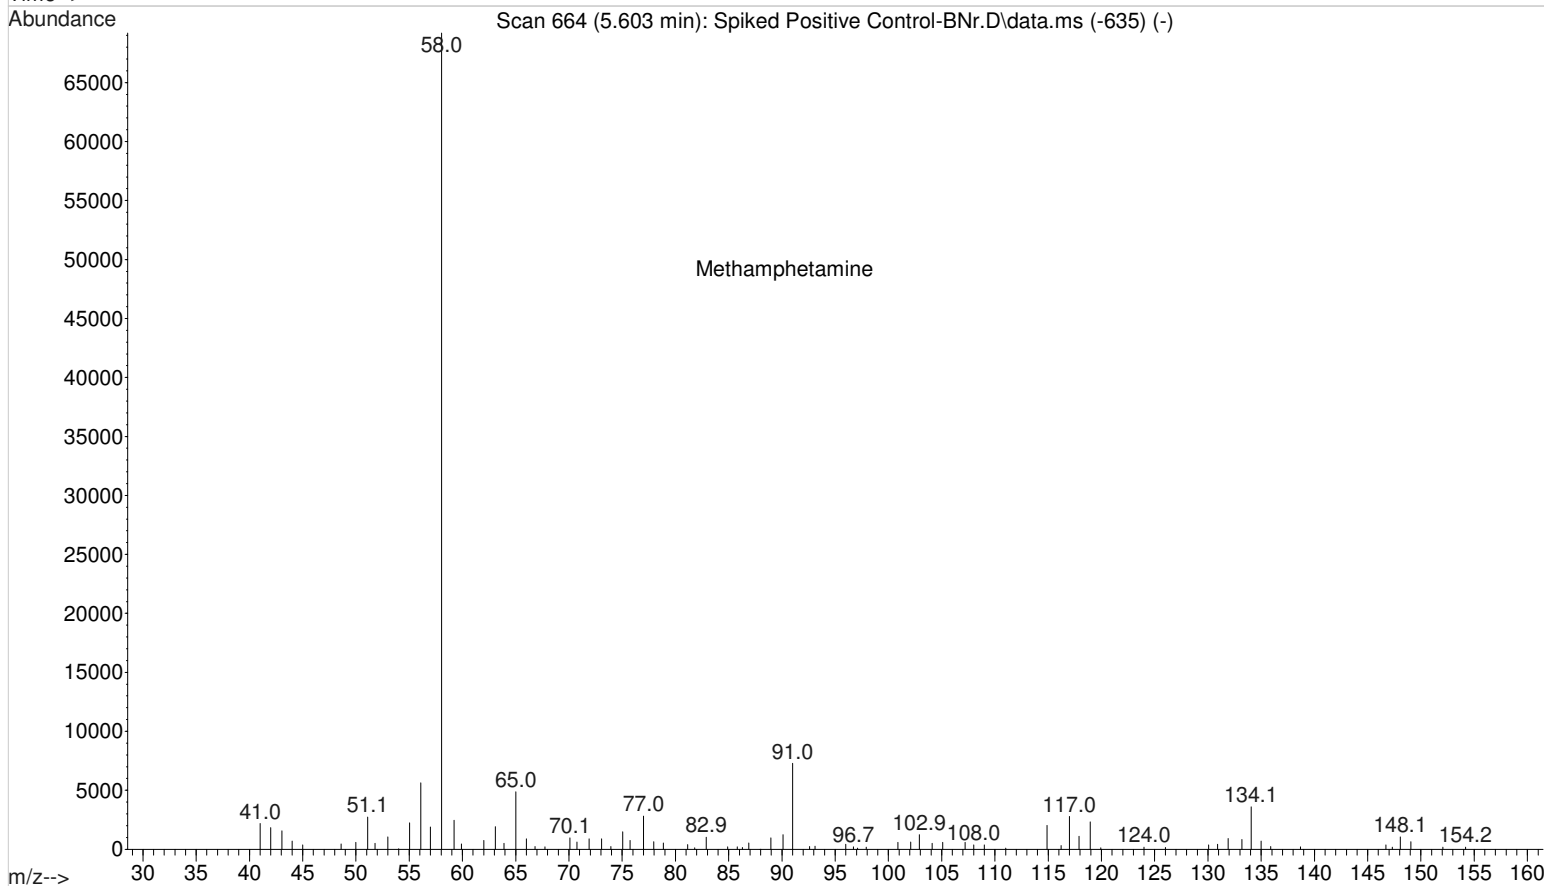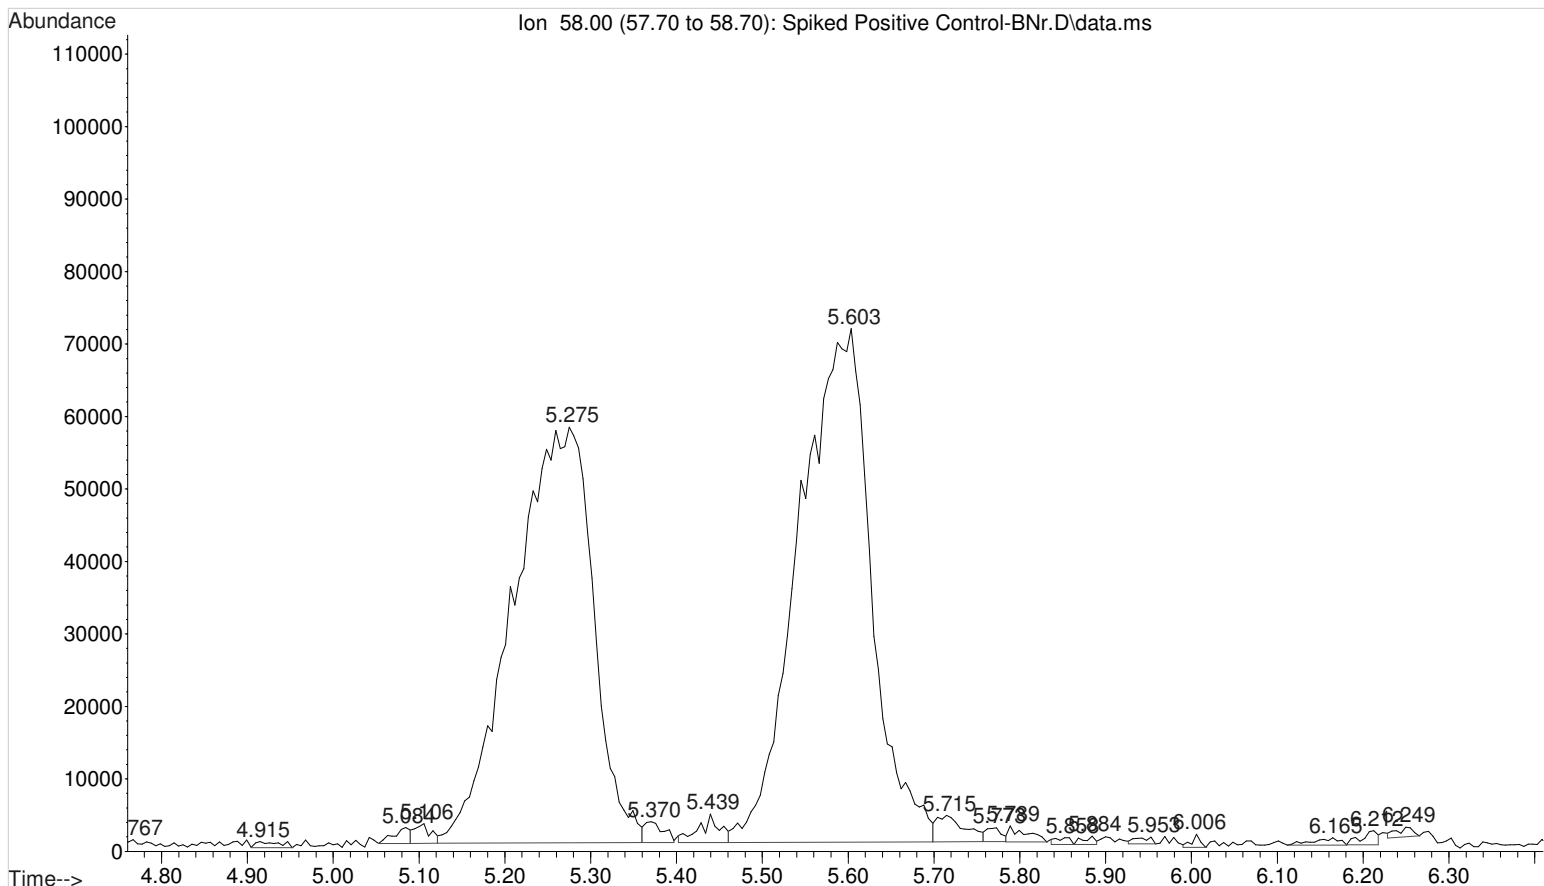

File : F:\10192016\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 19 Oct 2016 14:23 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

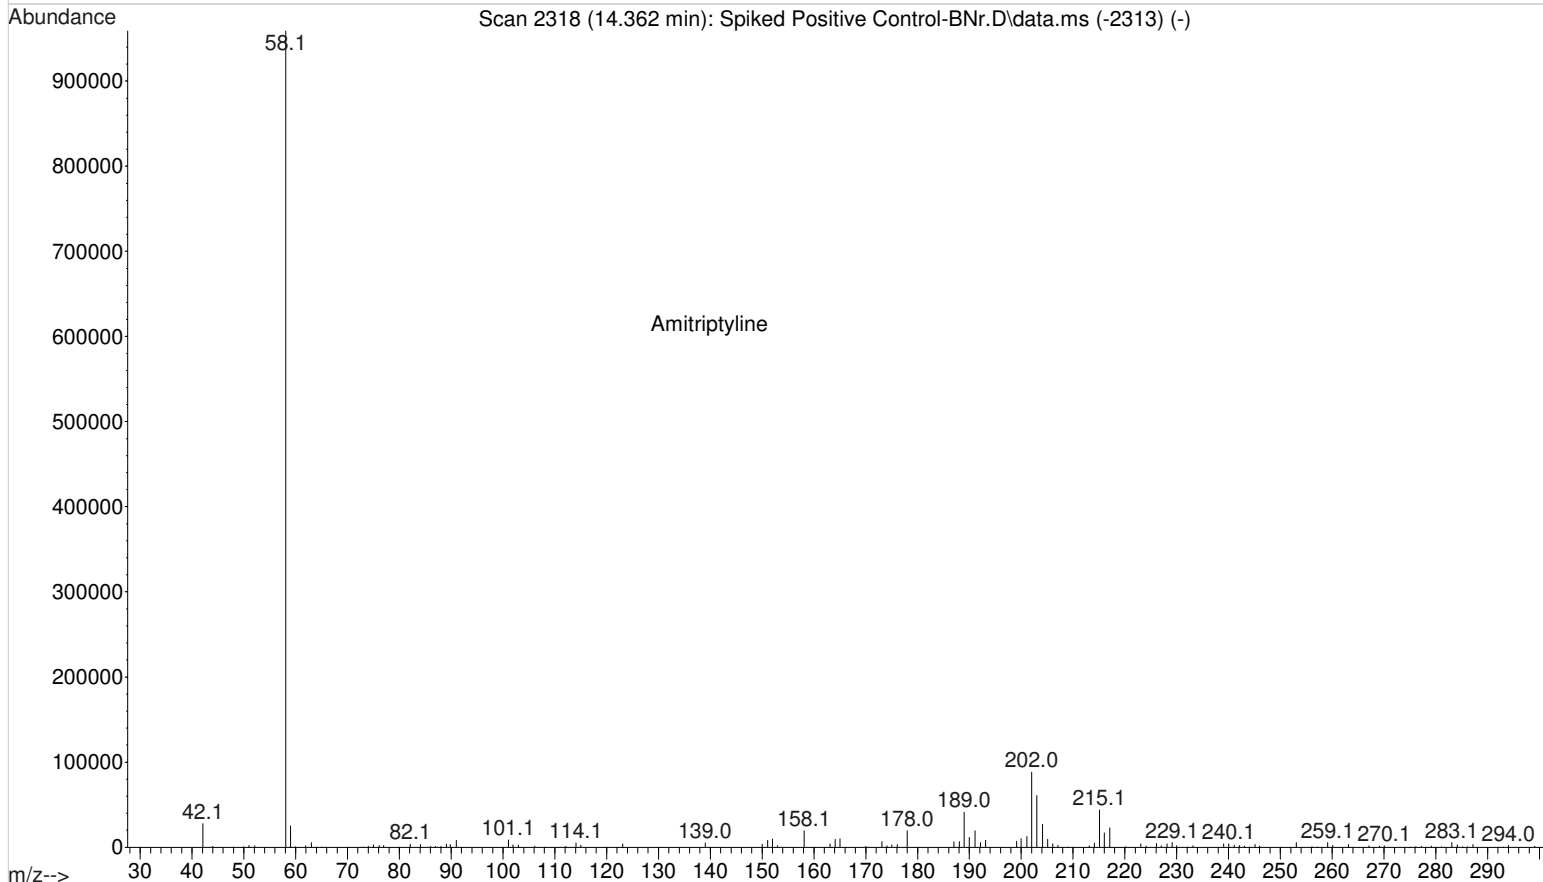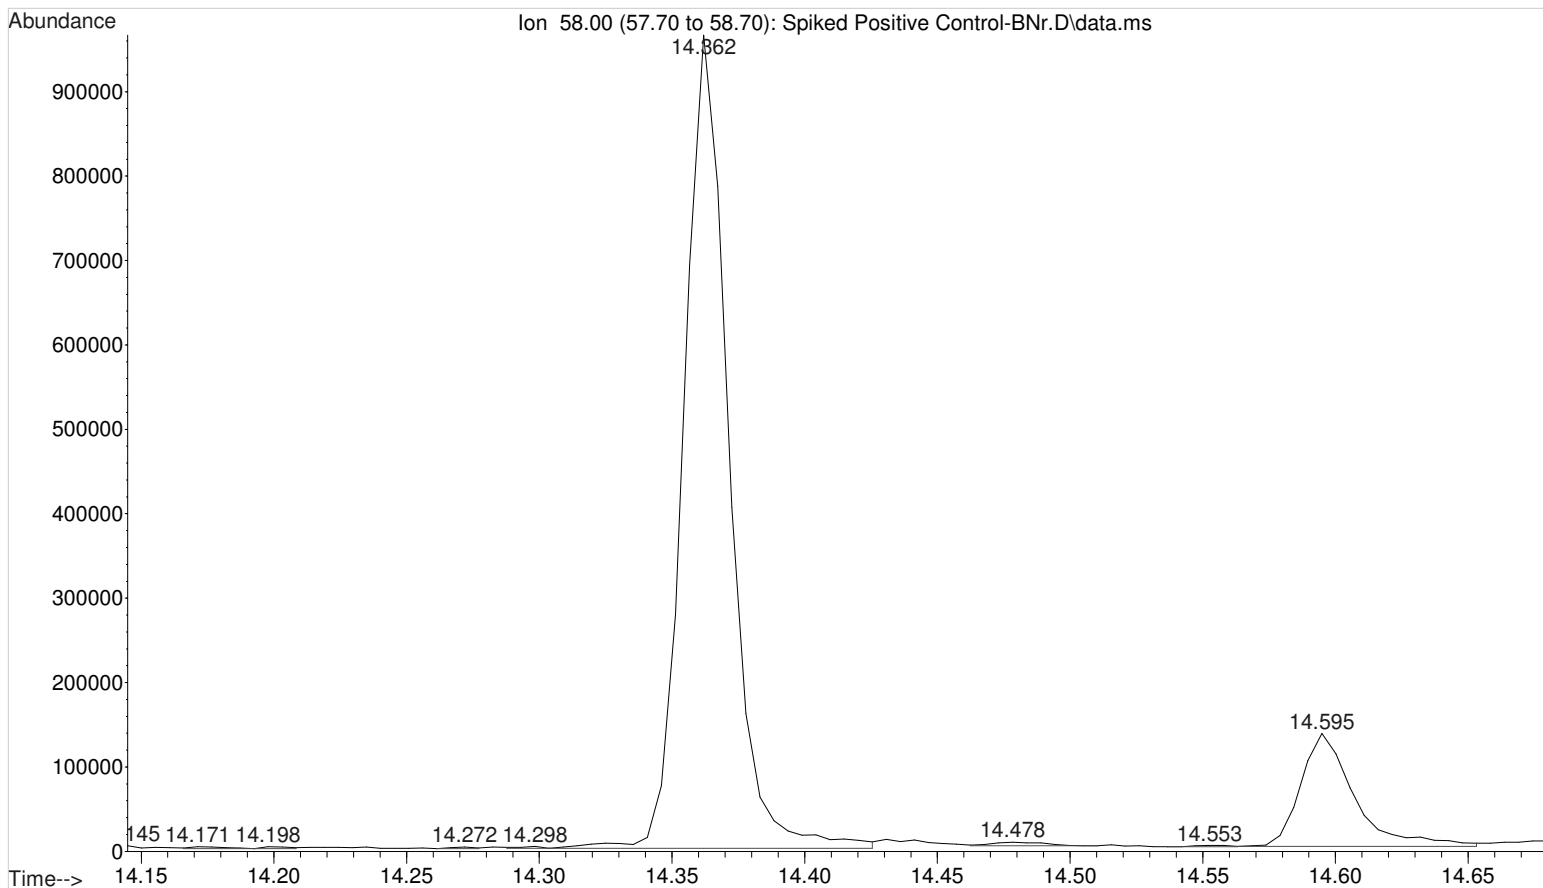

File : F:\10192016\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 19 Oct 2016 14:23 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

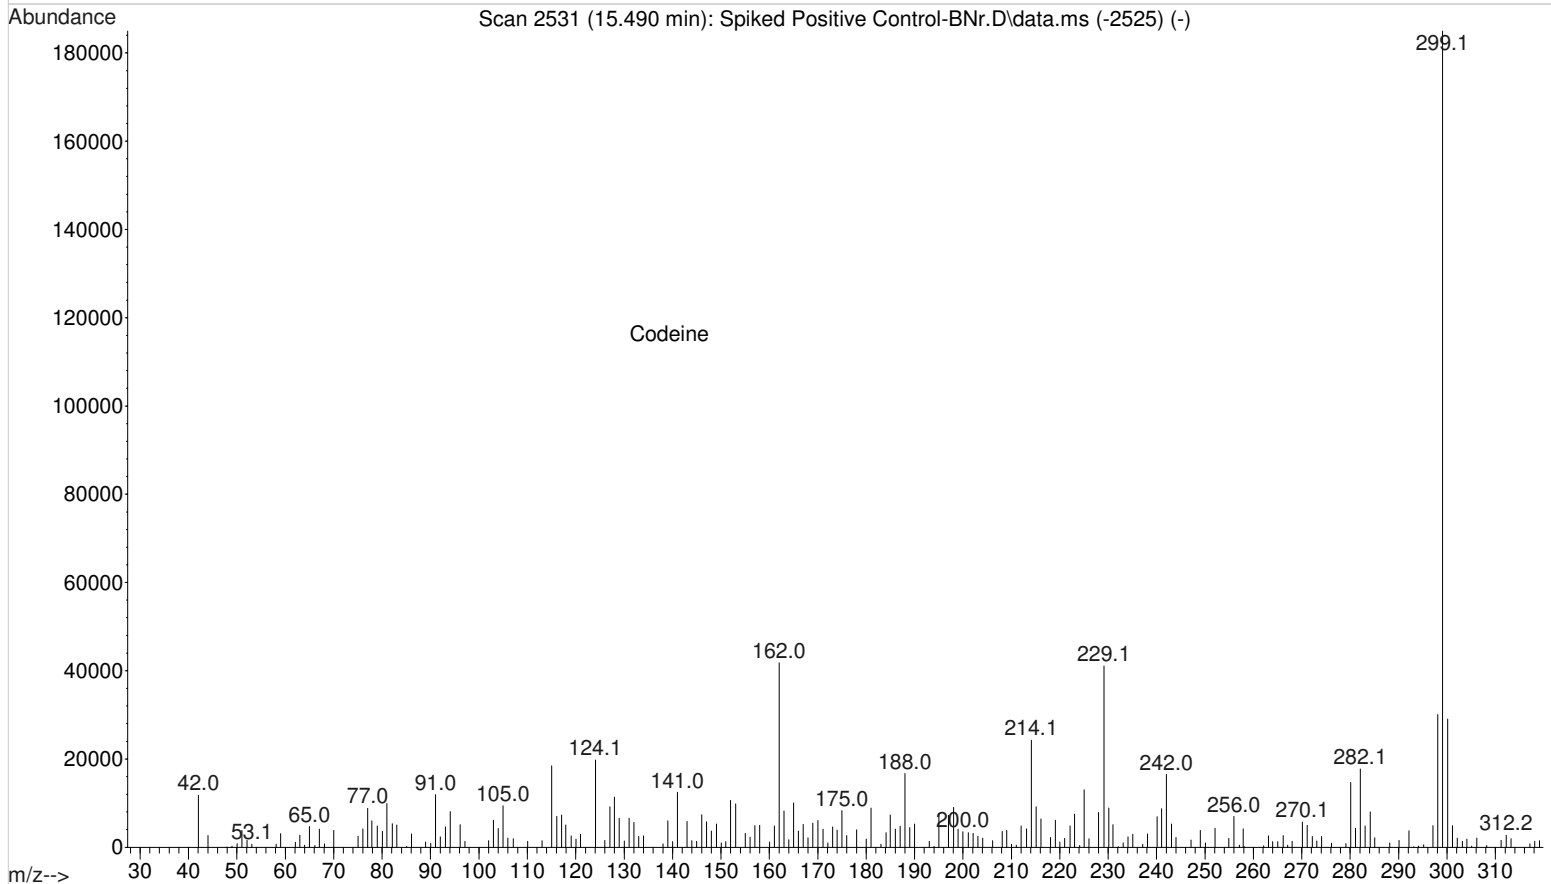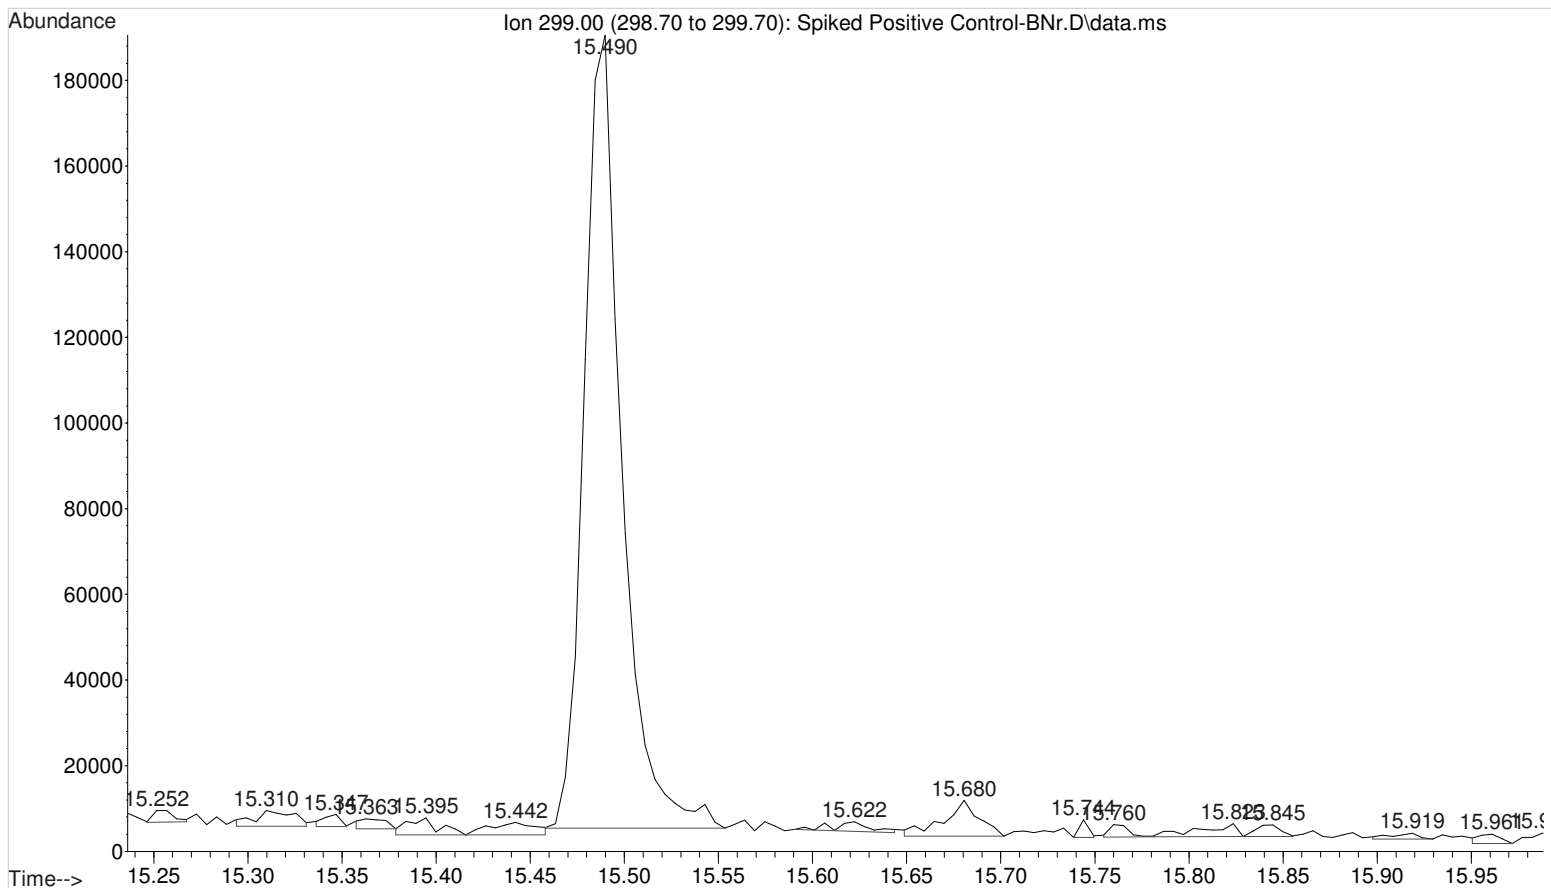

File : F:\10192016\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 19 Oct 2016 14:23 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name : Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

