























B. Wylie *[Signature]*

Worklist: 1342

<u>LAB_CASE</u>	<u>ITEM</u>	<u>TASK_ID</u>	<u>DESCRIPTION</u>	
C2016-0787	1	56131	AM 8 Blood base neutral confir	
C2016-0887	1	56998	AM 8 Blood base neutral confir	
C2016-1167	1	59189	AM 8 Blood base neutral confir	
C2016-1413	1	60854	AM 8 Blood base neutral confir	
M2016-1958	1	56406	AM 8 Blood base neutral confir	
M2016-2044	1	56741	AM 8 Blood base neutral confir	
M2016-2098	2	56987	AM 8 Blood base neutral confir	
M2016-3621	9	64248	AM 8 Blood base neutral confir	
P2016-1183	1	56623	AM 8 Blood base neutral confir	
P2016-1381	1	58294	AM 8 Blood base neutral confir	
P2016-1383	1	58301	AM 8 Blood base neutral confir	
P2016-1384	1	58304	AM 8 Blood base neutral confir	
P2016-1407	1	58467	AM 8 Blood base neutral confir	
P2016-1414	1	58486	AM 8 Blood base neutral confir	
P2016-1444	1	58648	AM 8 Blood base neutral confir	
P2016-1445	1	58664	AM 8 Blood base neutral confir	
P2016-1456	1	58749	AM 8 Blood base neutral confir	
P2016-1458	1	58793	AM 8 Blood base neutral confir	
P2016-1489	1	58968	AM 8 Blood base neutral confir	
P2016-1508	1	59082	AM 8 Blood base neutral confir	
P2016-1509	1	59085	AM 8 Blood base neutral confir	
P2016-1510	1	59088	AM 8 Blood base neutral confir	
P2016-1512	1	59135	AM 8 Blood base neutral confir	

Worklist: 1342



<u>LAB CASE</u>	<u>ITEM</u>	<u>TASK ID</u>	<u>DESCRIPTION</u>
P2016-1549	1	59481	AM 8 Blood base neutral confir
P2016-1563	1	59526	AM 8 Blood base neutral confir



Reviewed 11/8/16



Verified sequence
11/8/16 thn

simulate_sequence.log
Simulate Run Sequence Mon Nov 07 11:25:53 2016

Instrument Name: Major Mass Spec
Sequence File: C:\Users\ISPuser\Desktop\Sequences\tm-blanks.sequence.xml
Comment: MassHunter sequence
Operator: ISP\datastor
Data Path: D:\DATA\TM\2016\11072016\
Method Path: C:\Users\datastor\Desktop\OP Methods\

Line	Type	Vials	DataFile	Sample Name
Acquisition Method: BNSB120510.M				
1)	Sample	100	Prerun solvent blank	Pre-run Solvent Blank
2)	Sample	✓ 1	Negative Control-BN	Negative Control -
...1013				
3)	Sample	✓ 2	Spiked Positive Control-BN	Positive Control
4)	Sample	✓ 99	prBLK2	Solvent Blank
Acquisition Method: GBT092509-Delta EMV.M				
5)	Sample	100	Prerun Solvent blankr	Pre-run Solvent Blank
6)	Sample	✓ 1	Negative Control-BNr	Negative Control -
...1013				
7)	Sample	✓ 2	Spiked Positive Control-BNr	Positive Control
8)	Sample	99	prBLK2r	Solvent Blank
Acquisition Method: BNSB120510.M				
9)	Sample	100	C2016-0787-1-BNBLK	Lab No.: C2016-0787-1
10)	Sample	✓ 3	C2016-0787-1-BN	Lab No.: C2016-0787-1
Acquisition Method: GBT092509-Delta EMV.M				
11)	Sample	✓ 3	C2016-0787-1-BNr	Lab No.: C2016-0787-1
Acquisition Method: BNSB120510.M				
12)	Sample	100	C2016-0887-1-BNBLK	Lab No.: C2016-0887-1
13)	Sample	✓ 4	C2016-0887-1-BN	Lab No.: C2016-0887-1
Acquisition Method: GBT092509-Delta EMV.M				
14)	Sample	✓ 4	C2016-0887-1-BNr	Lab No.: C2016-0887-1
Acquisition Method: BNSB120510.M				
15)	Sample	100	C2016-1167-1-BNBLK	Lab No.: C2016-1167-1
16)	Sample	✓ 5	C2016-1167-1-BN	Lab No.: C2016-1167-1
Acquisition Method: GBT092509-Delta EMV.M				
17)	Sample	✓ 5	C2016-1167-1-BNr	Lab No.: C2016-1167-1
Acquisition Method: BNSB120510.M				
18)	Sample	100	C2016-1413-1-BNBLK	Lab No.: C2016-1413-1
19)	Sample	✓ 6	C2016-1413-1-BN	Lab No.: C2016-1413-1
Acquisition Method: GBT092509-Delta EMV.M				
20)	Sample	✓ 6	C2016-1413-1-BNr	Lab No.: C2016-1413-1
Acquisition Method: BNSB120510.M				
21)	Sample	100	M2016-1958-1-BNBLK	Lab No.: M2016-1958-1
22)	Sample	✓ 7	M2016-1958-1-BN	Lab No.: M2016-1958-1
Acquisition Method: GBT092509-Delta EMV.M				
23)	Sample	✓ 7	M2016-1958-1-BNr	Lab No.: M2016-1958-1
Acquisition Method: BNSB120510.M				
24)	Sample	100	M2016-2044-1-BNBLK	Lab No.: M2016-2044-1
25)	Sample	✓ 8	M2016-2044-1-BN	Lab No.: M2016-2044-1
Acquisition Method: GBT092509-Delta EMV.M				
26)	Sample	✓ 8	M2016-2044-1-BNr	Lab No.: M2016-2044-1

simulate_sequence.log

Acquisition Method:	BNSB120510.M		
27) Sample	100	M2016-2098-2-BNBLK	Lab No.: M2016-2098-2
28) Sample	✓ 9	M2016-2098-2-BN	Lab No.: M2016-2098-2
Acquisition Method:	GBT092509-Delta EMV.M		
29) Sample	✓ 9	M2016-2098-2-BNr	Lab No.: M2016-2098-2
Acquisition Method:	BNSB120510.M		
30) Sample	100	M2016-3621-9-BNBLK	Lab No.: M2016-3621-9
31) Sample	✓ 10	M2016-3621-9-BN	Lab No.: M2016-3621-9
Acquisition Method:	GBT092509-Delta EMV.M		
32) Sample	✓ 10	M2016-3621-9-BNr	Lab No.: M2016-3621-9
Acquisition Method:	BNSB120510.M		
33) Sample	100	P2016-1183-1-BNBLK	Lab No.: P2016-1183-1
34) Sample	✓ 11	P2016-1183-1-BN	Lab No.: P2016-1183-1
Acquisition Method:	GBT092509-Delta EMV.M		
35) Sample	✓ 11	P2016-1183-1-BNr	Lab No.: P2016-1183-1
Acquisition Method:	BNSB120510.M		
36) Sample	100	P2016-1381-1-BNBLK	Lab No.: P2016-1381-1
37) Sample	✓ 12	P2016-1381-1-BN	Lab No.: P2016-1381-1
Acquisition Method:	GBT092509-Delta EMV.M		
38) Sample	✓ 12	P2016-1381-1-BNr	Lab No.: P2016-1381-1
Acquisition Method:	BNSB120510.M		
39) Sample	100	P2016-1383-1-BNBLK	Lab No.: P2016-1383-1
40) Sample	✓ 13	P2016-1383-1-BN	Lab No.: P2016-1383-1
Acquisition Method:	GBT092509-Delta EMV.M		
41) Sample	✓ 13	P2016-1383-1-BNr	Lab No.: P2016-1383-1
Acquisition Method:	BNSB120510.M		
42) Sample	100	P2016-1384-1-BNBLK	Lab No.: P2016-1384-1
43) Sample	✓ 14	P2016-1384-1-BN	Lab No.: P2016-1384-1
Acquisition Method:	GBT092509-Delta EMV.M		
44) Sample	✓ 14	P2016-1384-1-BNr	Lab No.: P2016-1384-1
Acquisition Method:	BNSB120510.M		
45) Sample	100	P2016-1407-1-BNBLK	Lab No.: P2016-1407-1
46) Sample	✓ 15	P2016-1407-1-BN	Lab No.: P2016-1407-1
Acquisition Method:	GBT092509-Delta EMV.M		
47) Sample	✓ 15	P2016-1407-1-BNr	Lab No.: P2016-1407-1
Acquisition Method:	BNSB120510.M		
48) Sample	✓ 99	P2016-1414-1-BNBLK	Lab No.: P2016-1414-1
49) Sample	✓ 16	P2016-1414-1-BN	Lab No.: P2016-1414-1
Acquisition Method:	GBT092509-Delta EMV.M		
50) Sample	✓ 16	P2016-1414-1-BNr	Lab No.: P2016-1414-1
Acquisition Method:	BNSB120510.M		
51) Sample	✓ 99	P2016-1444-1-BNBLK	Lab No.: P2016-1444-1
52) Sample	✓ 17	P2016-1444-1-BN	Lab No.: P2016-1444-1
Acquisition Method:	GBT092509-Delta EMV.M		
53) Sample	✓ 17	P2016-1444-1-BNr	Lab No.: P2016-1444-1
Acquisition Method:	BNSB120510.M		
54) Sample	✓ 99	P2016-1445-1-BNBLK	Lab No.: P2016-1445-1
55) Sample	✓ 18	P2016-1445-1-BN	Lab No.: P2016-1445-1


simulate_sequence.log

Acquisition Method: GBT092509-Delta EMV.M			
56) Sample	✓ 18	P2016-1445-1-BNr	Lab No.: P2016-1445-1
Acquisition Method: BNSB120510.M			
57) Sample	✓ 99	P2016-1456-1-BNBLK	Lab No.: P2016-1456-1
58) Sample	✓ 19	P2016-1456-1-BN	Lab No.: P2016-1456-1
Acquisition Method: GBT092509-Delta EMV.M			
59) Sample	✓ 19	P2016-1456-1-BNr	Lab No.: P2016-1456-1
Acquisition Method: BNSB120510.M			
60) Sample	✓ 99	P2016-1458-1-BNBLK	Lab No.: P2016-1458-1
61) Sample	✓ 20	P2016-1458-1-BN	Lab No.: P2016-1458-1
Acquisition Method: GBT092509-Delta EMV.M			
62) Sample	✓ 20	P2016-1458-1-BNr	Lab No.: P2016-1458-1
Acquisition Method: BNSB120510.M			
63) Sample	✓ 99	P2016-1489-1-BNBLK	Lab No.: P2016-1489-1
64) Sample	✓ 21	P2016-1489-1-BN	Lab No.: P2016-1489-1
Acquisition Method: GBT092509-Delta EMV.M			
65) Sample	✓ 21	P2016-1489-1-BNr	Lab No.: P2016-1489-1
Acquisition Method: BNSB120510.M			
66) Sample	✓ 99	P2016-1508-1-BNBLK	Lab No.: P2016-1508-1
67) Sample	✓ 22	P2016-1508-1-BN	Lab No.: P2016-1508-1
Acquisition Method: GBT092509-Delta EMV.M			
68) Sample	✓ 22	P2016-1508-1-BNr	Lab No.: P2016-1508-1
Acquisition Method: BNSB120510.M			
69) Sample	✓ 99	P2016-1509-1-BNBLK	Lab No.: P2016-1509-1
70) Sample	✓ 23	P2016-1509-1-BN	Lab No.: P2016-1509-1
Acquisition Method: GBT092509-Delta EMV.M			
71) Sample	✓ 23	P2016-1509-1-BNr	Lab No.: P2016-1509-1
Acquisition Method: BNSB120510.M			
72) Sample	✓ 99	P2016-1510-1-BNBLK	Lab No.: P2016-1510-1
73) Sample	✓ 24	P2016-1510-1-BN	Lab No.: P2016-1510-1
Acquisition Method: GBT092509-Delta EMV.M			
74) Sample	✓ 24	P2016-1510-1-BNr	Lab No.: P2016-1510-1
Acquisition Method: BNSB120510.M			
75) Sample	✓ 99	P2016-1512-1-BNBLK	Lab No.: P2016-1512-1
76) Sample	✓ 25	P2016-1512-1-BN	Lab No.: P2016-1512-1
Acquisition Method: GBT092509-Delta EMV.M			
77) Sample	✓ 25	P2016-1512-1-BNr	Lab No.: P2016-1512-1
Acquisition Method: BNSB120510.M			
78) Sample	✓ 99	P2016-1549-1-BNBLK	Lab No.: P2016-1549-1
79) Sample	✓ 26	P2016-1549-1-BN	Lab No.: P2016-1549-1
Acquisition Method: GBT092509-Delta EMV.M			
80) Sample	✓ 26	P2016-1549-1-BNr	Lab No.: P2016-1549-1
Acquisition Method: BNSB120510.M			
81) Sample	✓ 99	P2016-1563-1-BNBLK	Lab No.: P2016-1563-1
82) Sample	✓ 27	P2016-1563-1-BN	Lab No.: P2016-1563-1
Acquisition Method: GBT092509-Delta EMV.M			
83) Sample	✓ 27	P2016-1563-1-BNr	Lab No.: P2016-1563-1
Acquisition Method: BNSB120510.M			
84) Sample	✓ 99	POSTBLK	BLK


simulate_sequence.log

Acquisition Method: ~~GBT092509-Delta~~ EMV.M
85) Sample ✓ 99 AFTER BLK
megabytes Needed: 1428 Space on drive D: 213879
Sequence Verification Done!


File :F:\11072016\Prerun Solvent Blank.D
Operator : ISP\datastor
Acquired : 07 Nov 2016 11:49 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Pre-run Solvent Blank
Misc Info : Chloroform
Vial Number: 100

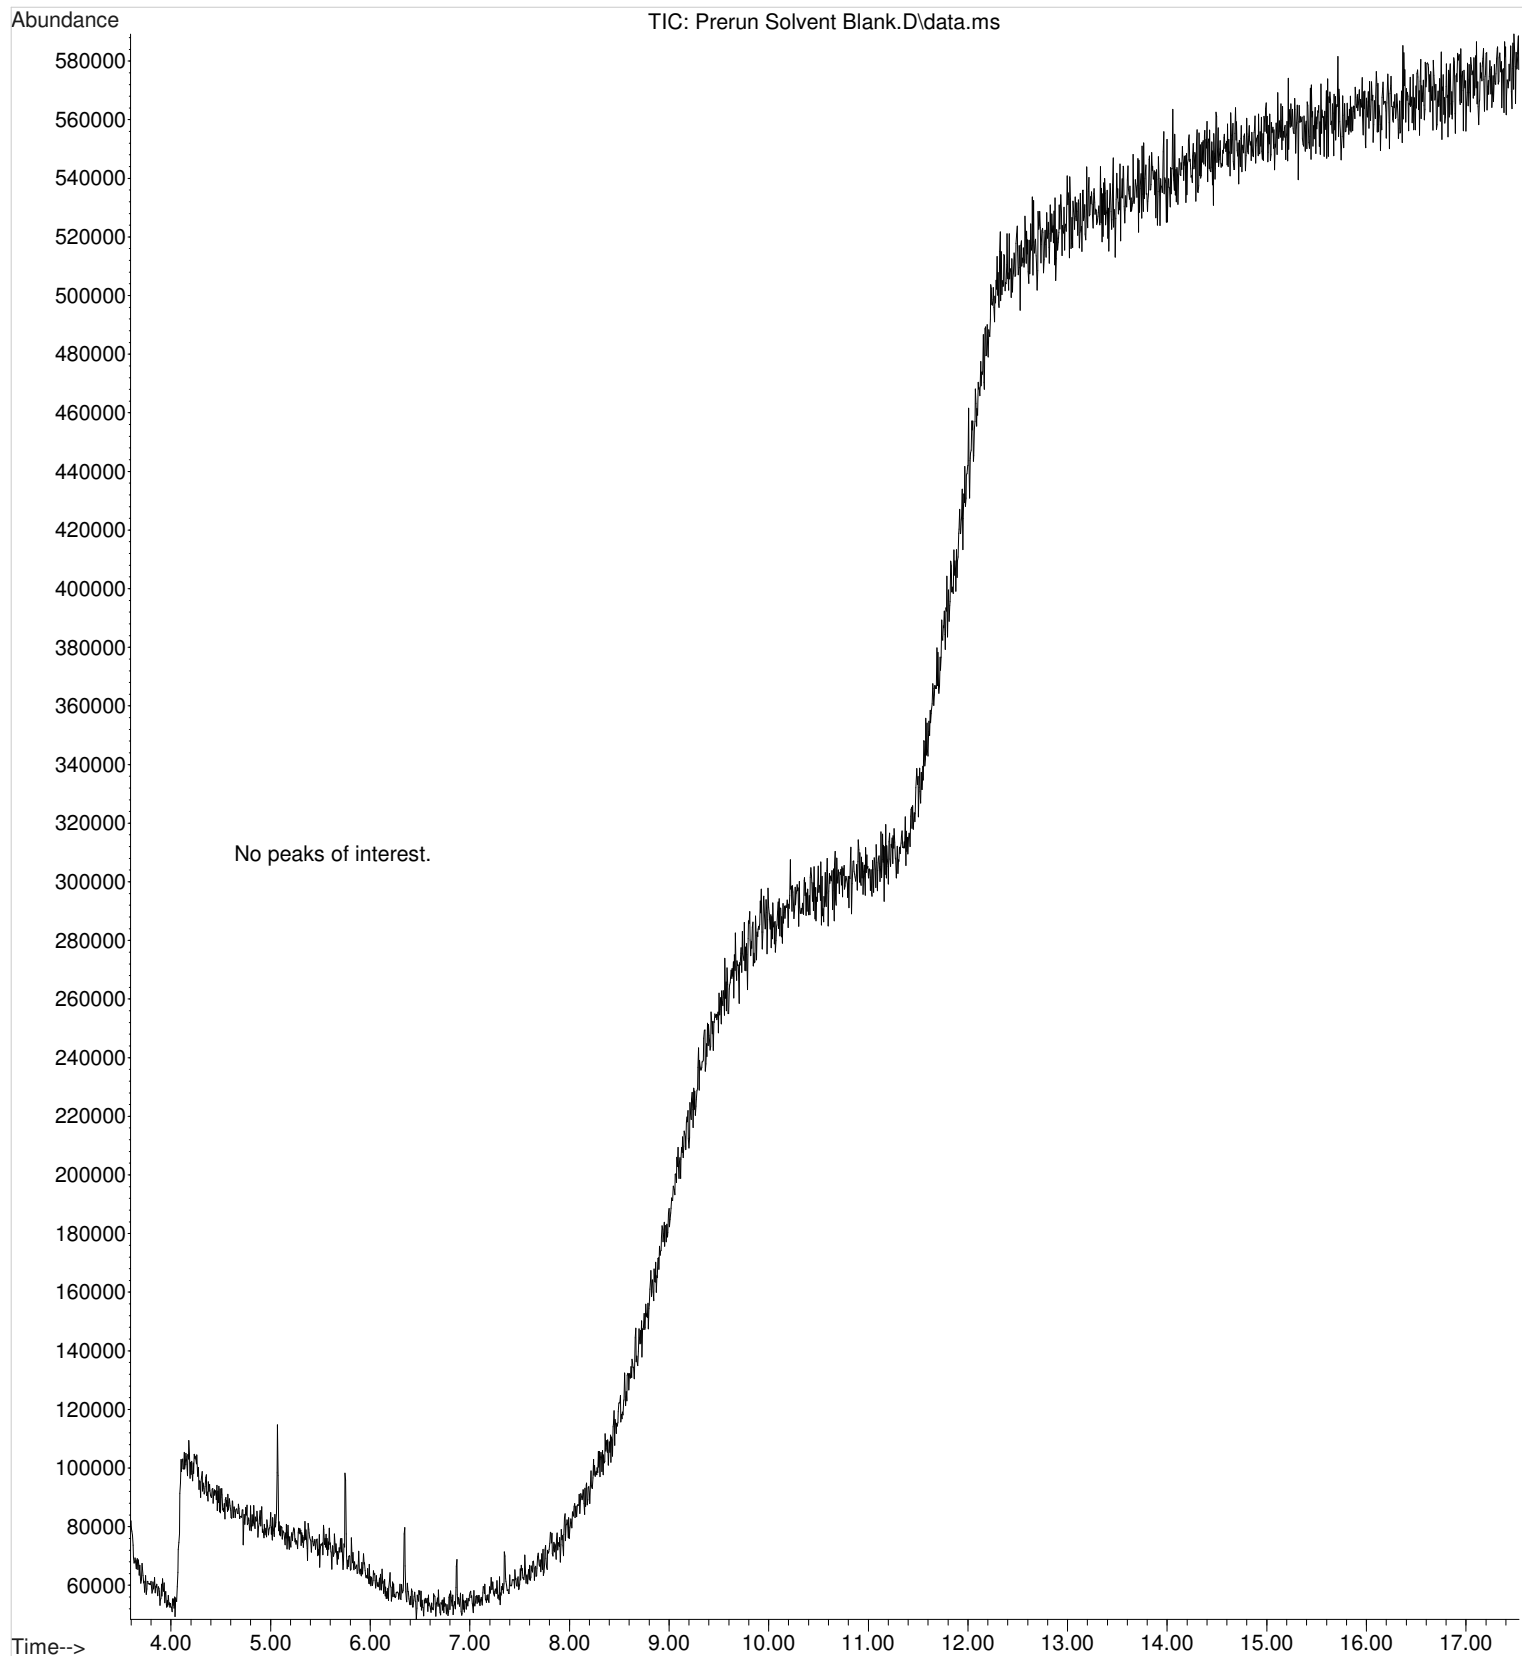



File :F:\11072016\prbLK2.D
Operator : ISP\datastor
Acquired : 07 Nov 2016 12:58 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Solvent Blank
Misc Info : Chloroform
Vial Number: 99

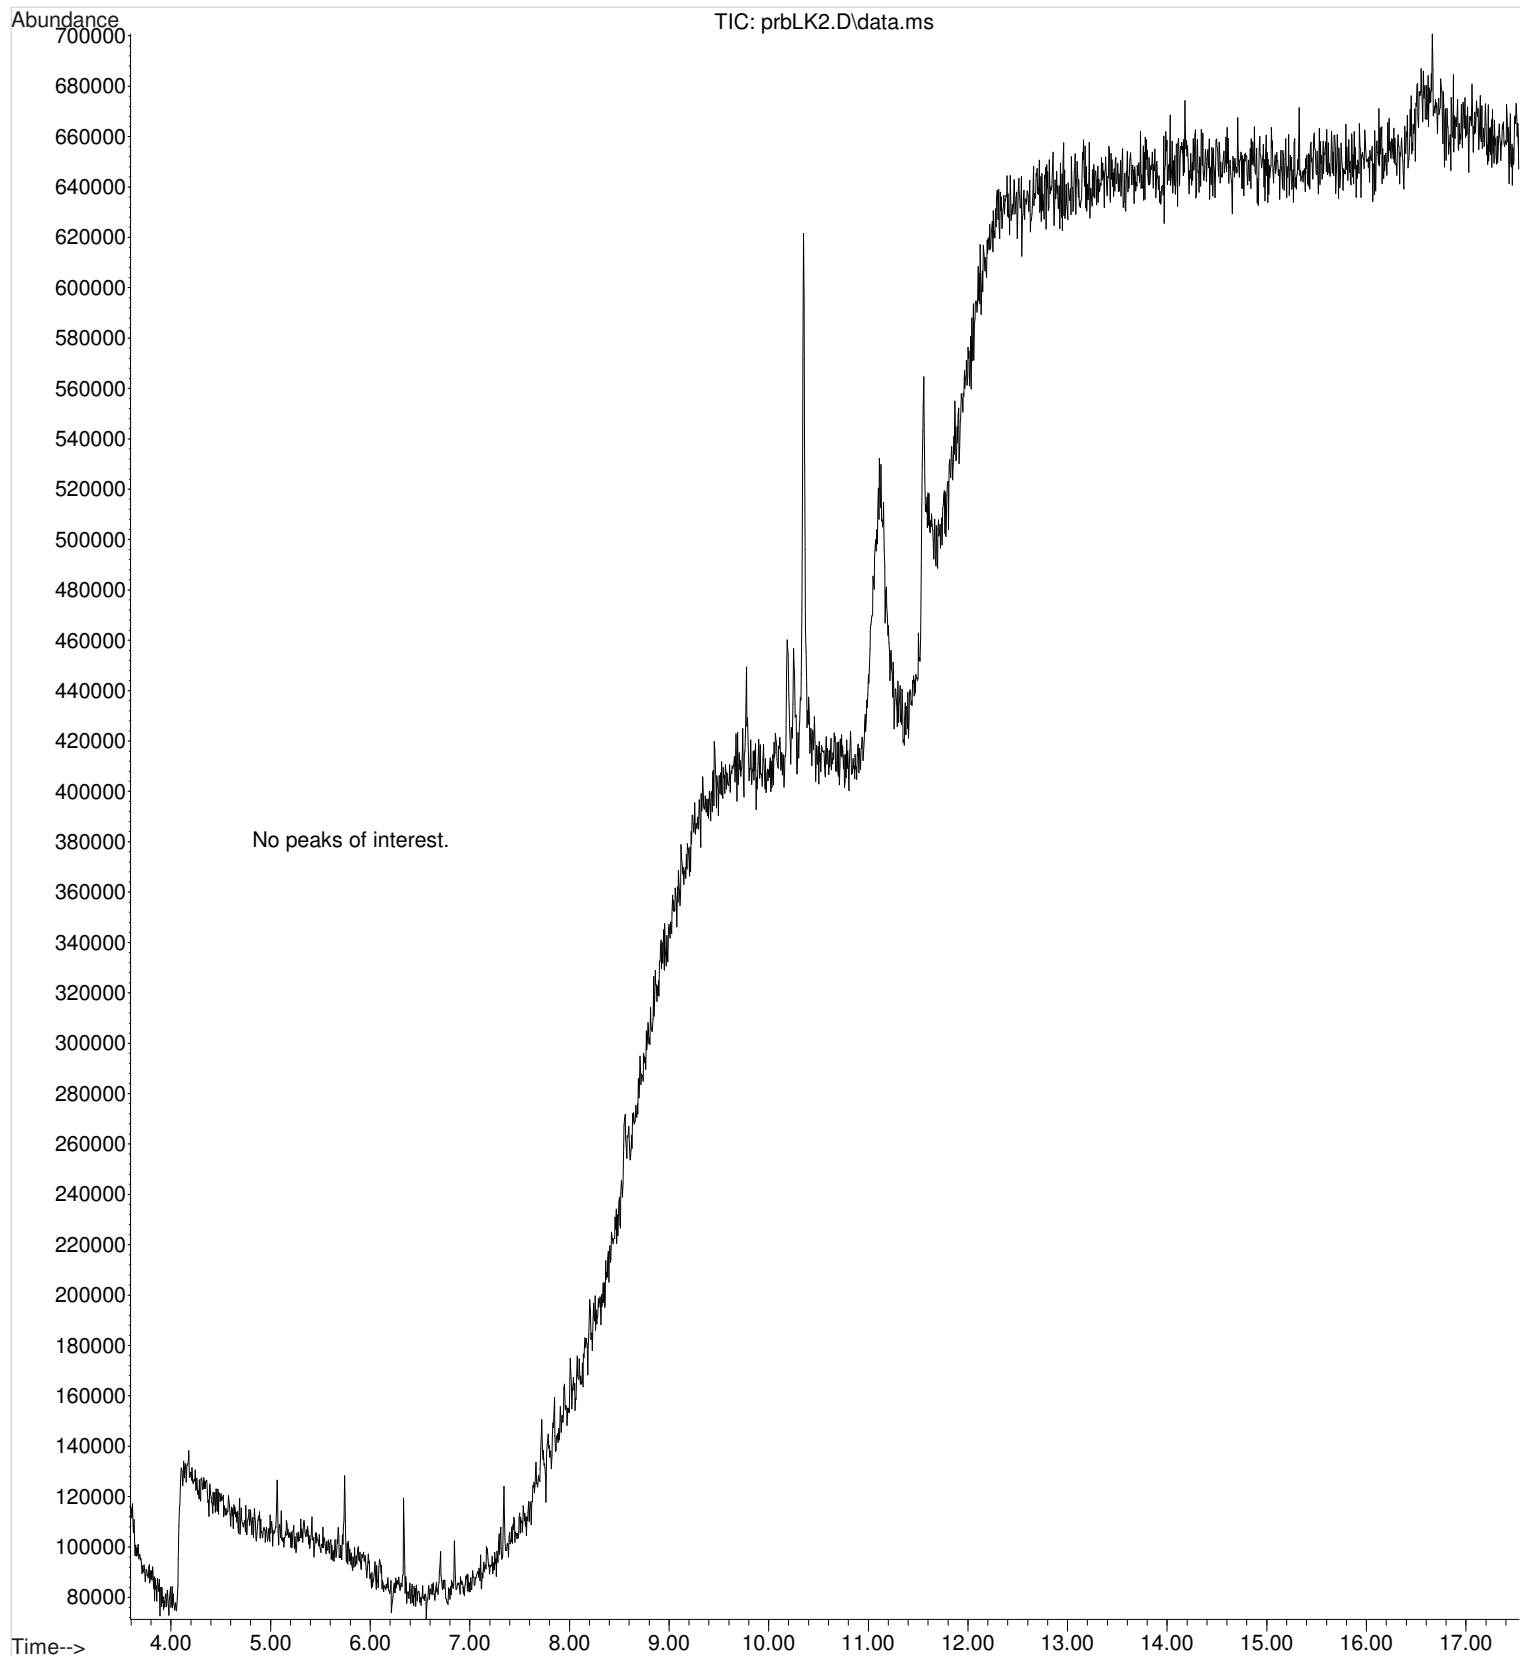



File :F:\11072016\Negative Control-BN.D
Operator : ISP\datastor
Acquired : 07 Nov 2016 12:12 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B1013
Misc Info : Analytical Method 3.6.1
Vial Number: 1

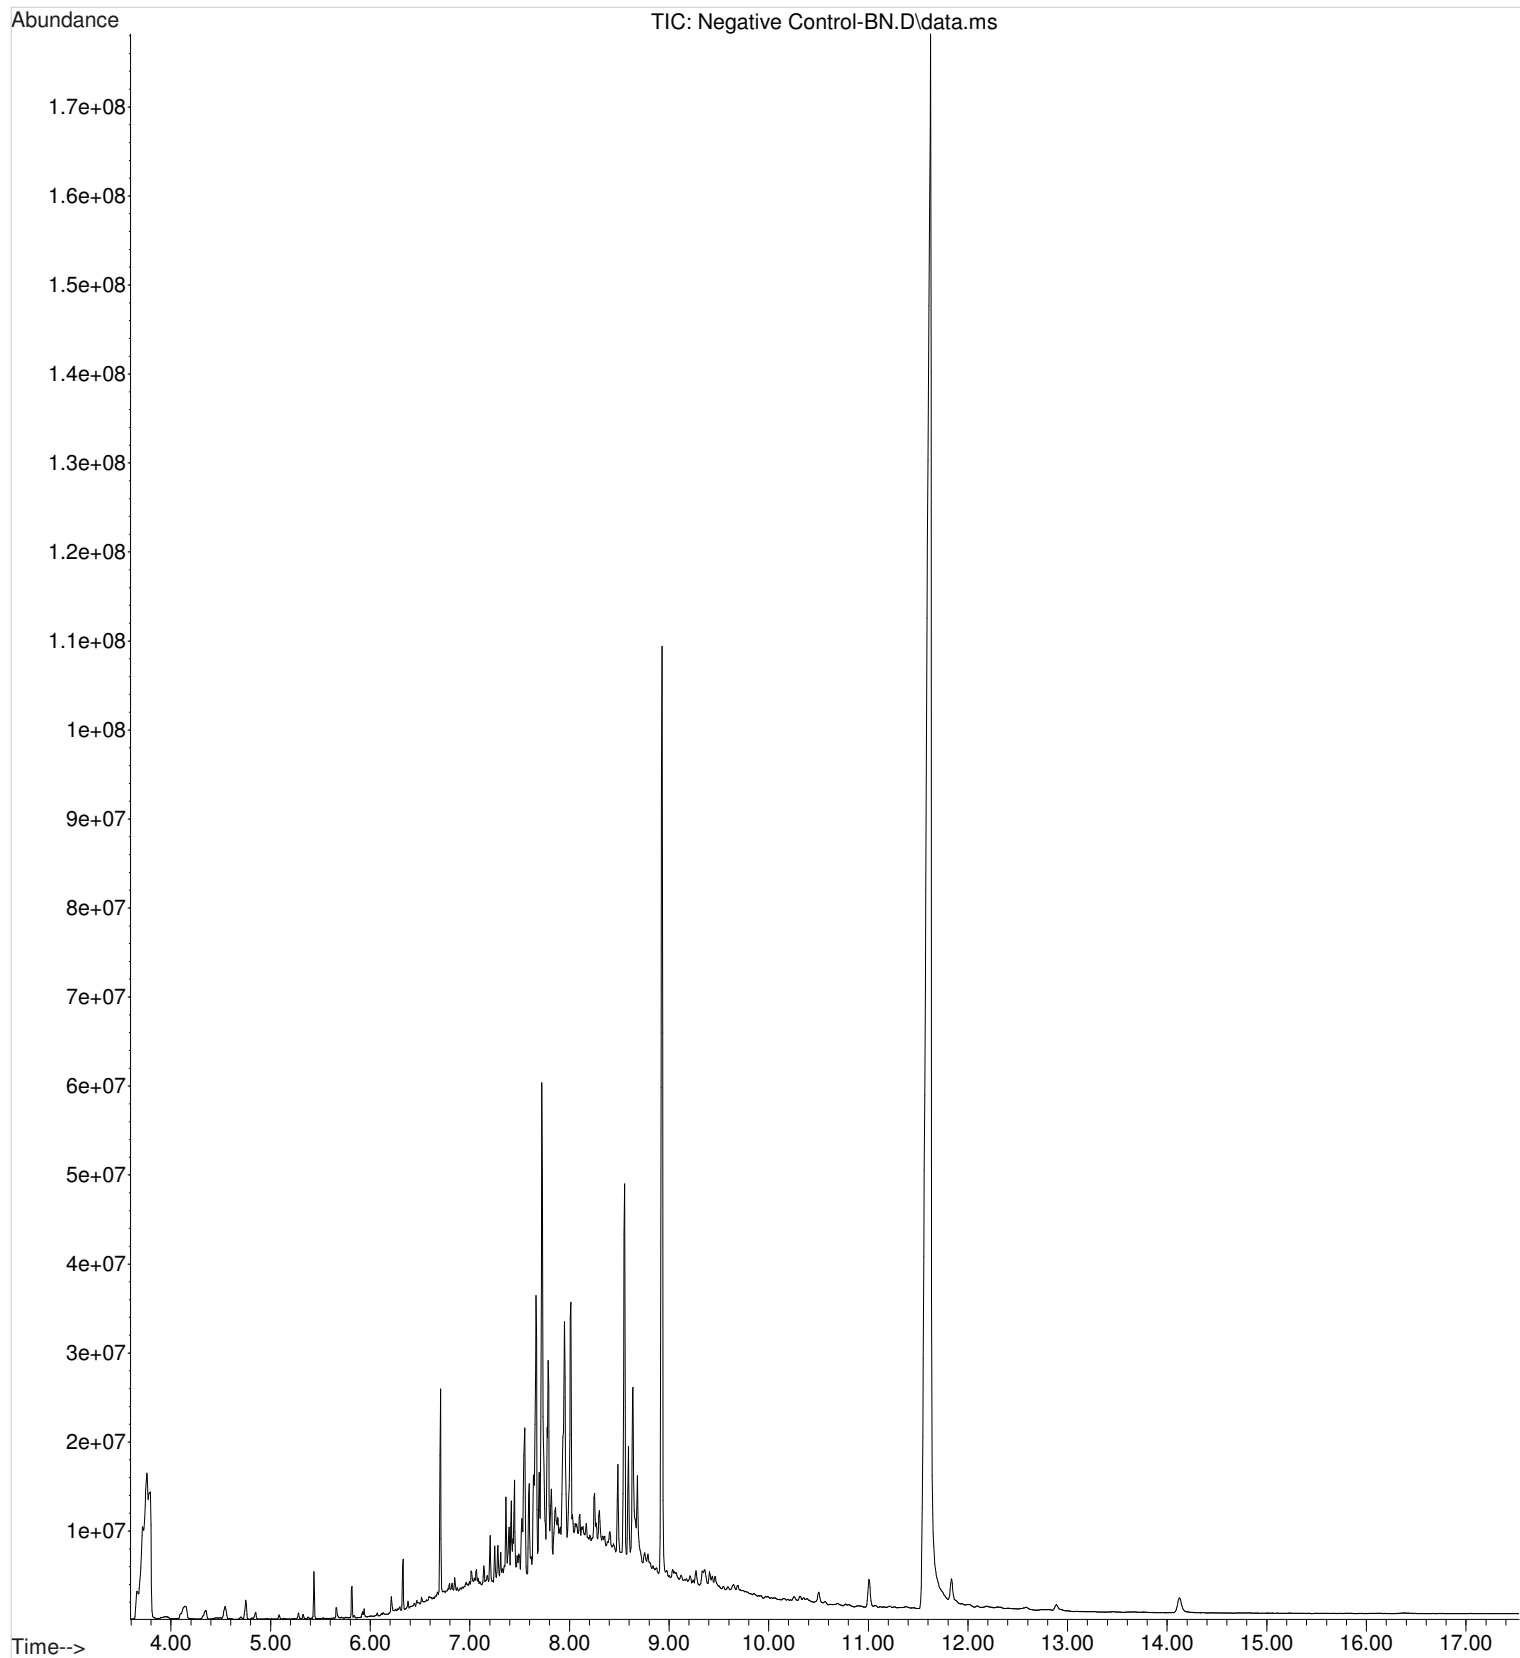


File : F:\11072016\Negative Control-BN.D
Operator : ISP\datastor
Acquired : 07 Nov 2016 12:12 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name : Negative Control - Utak Lot B1013
Misc Info : Analytical Method 3.6.1
Vial Number: 1

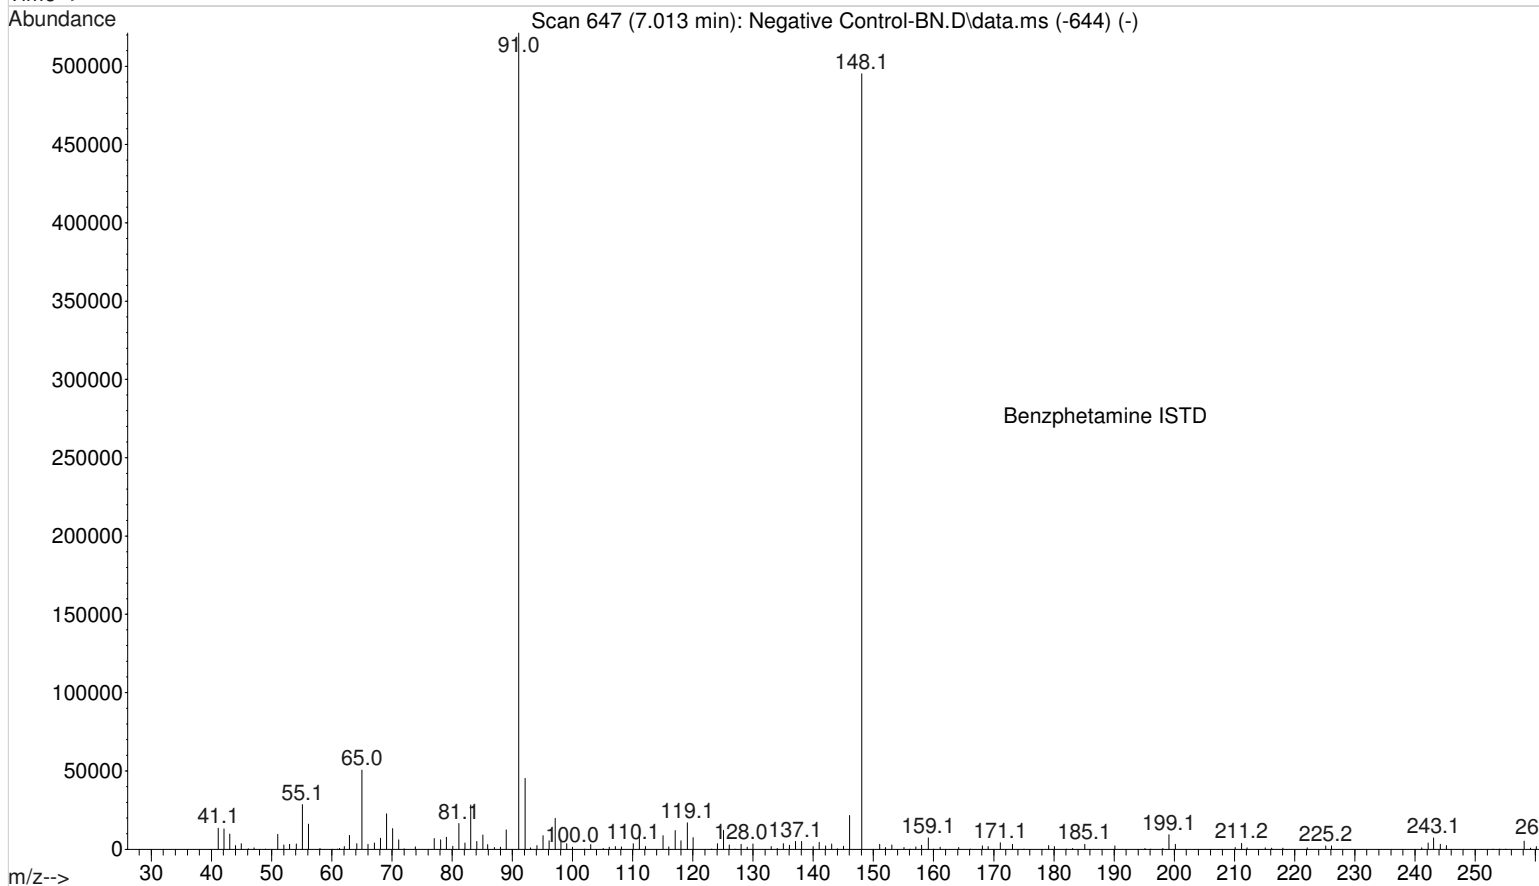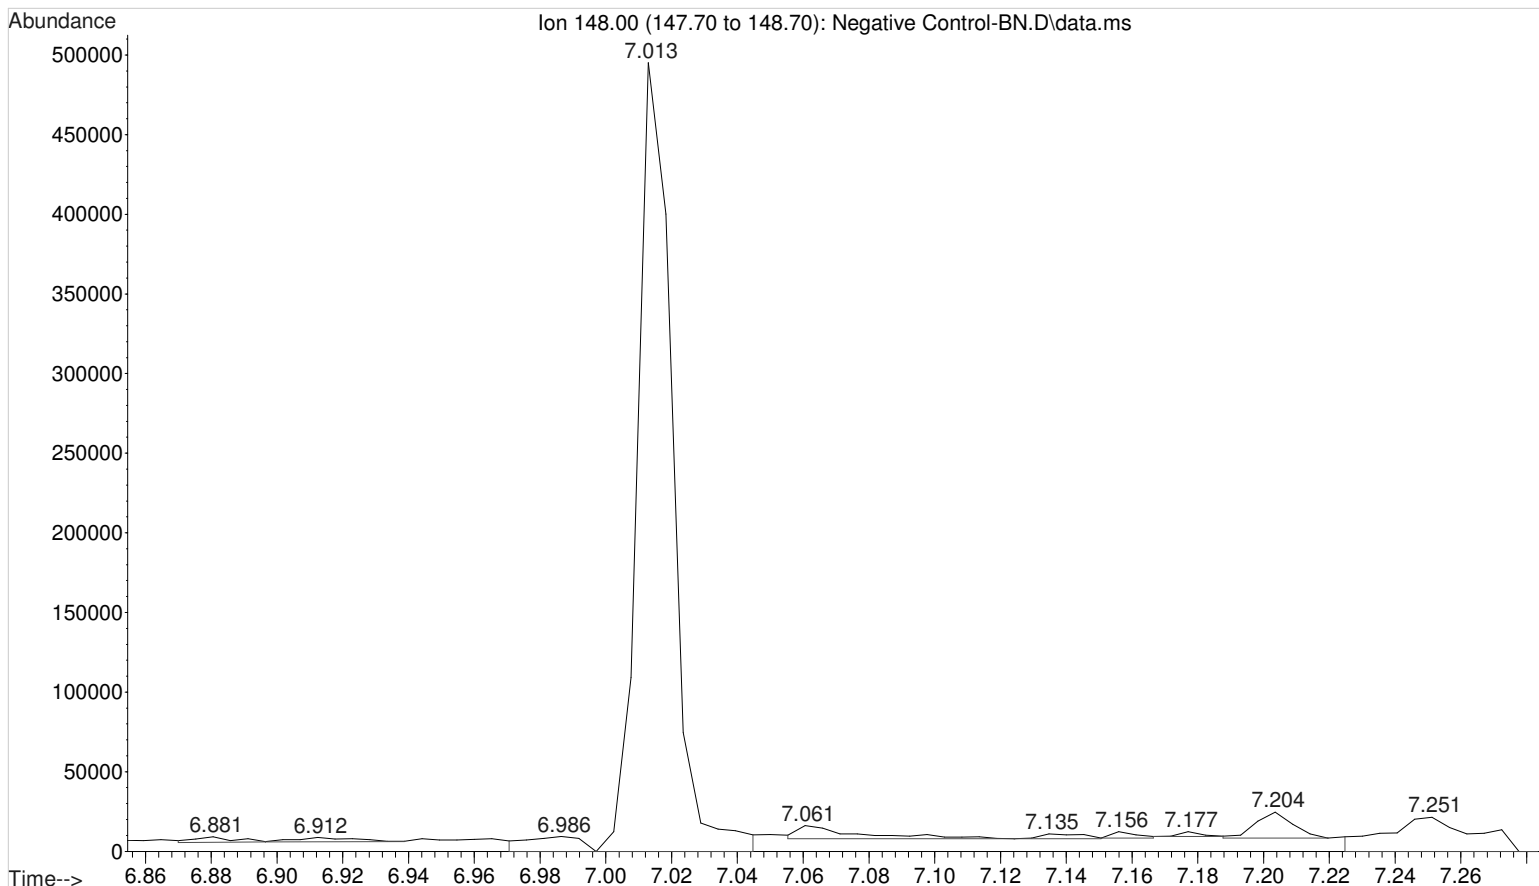



File : F:\11072016\Negative Control-BN.D
Operator : ISP\datastor
Acquired : 07 Nov 2016 12:12 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name : Negative Control - Utak Lot B1013
Misc Info : Analytical Method 3.6.1
Vial Number: 1

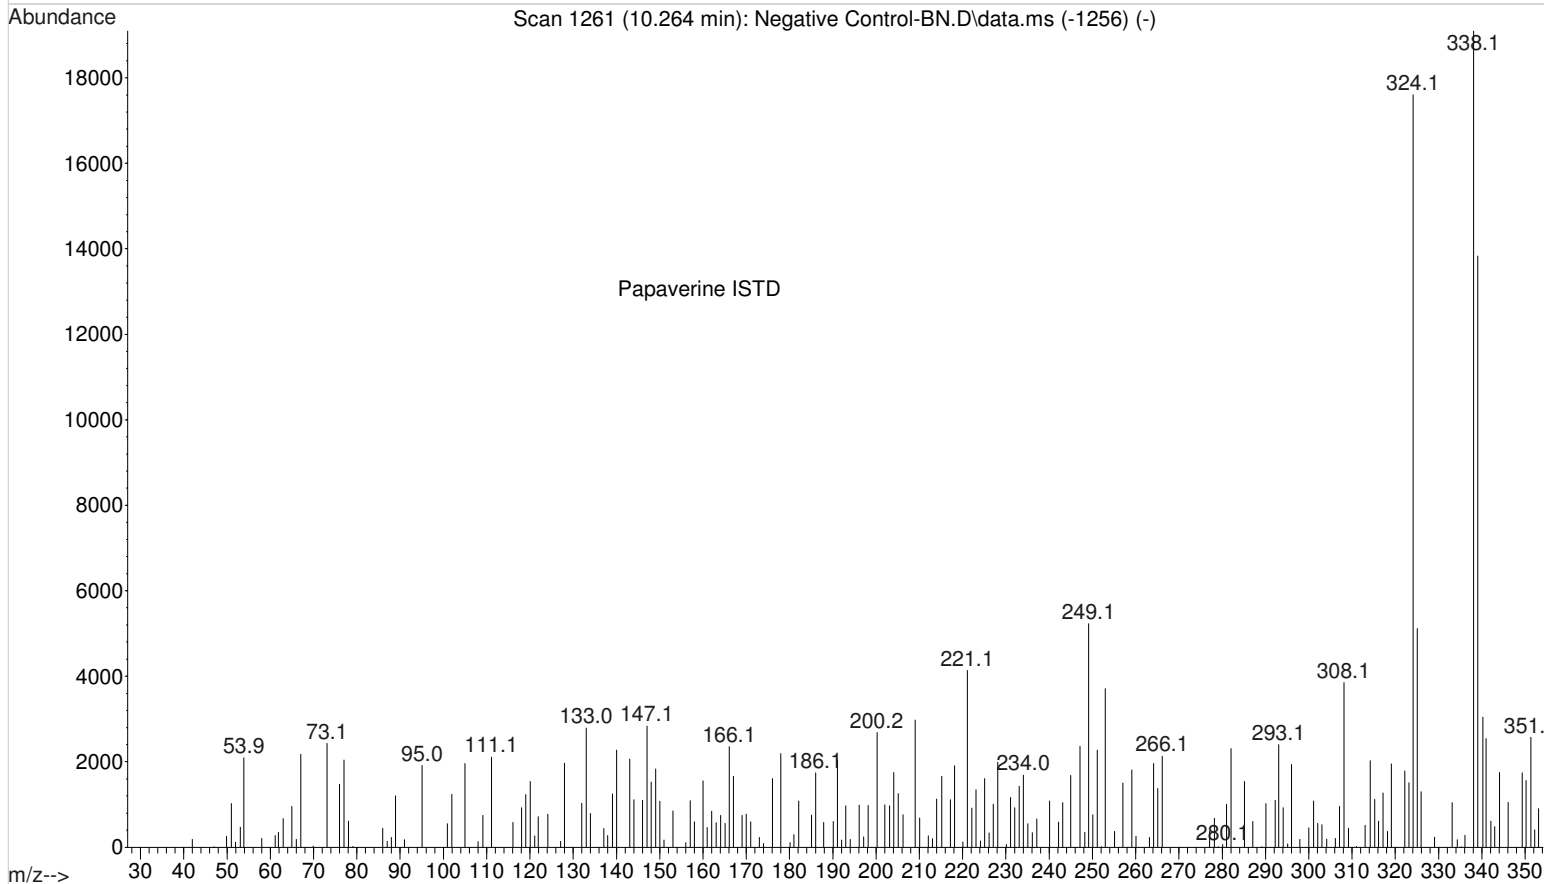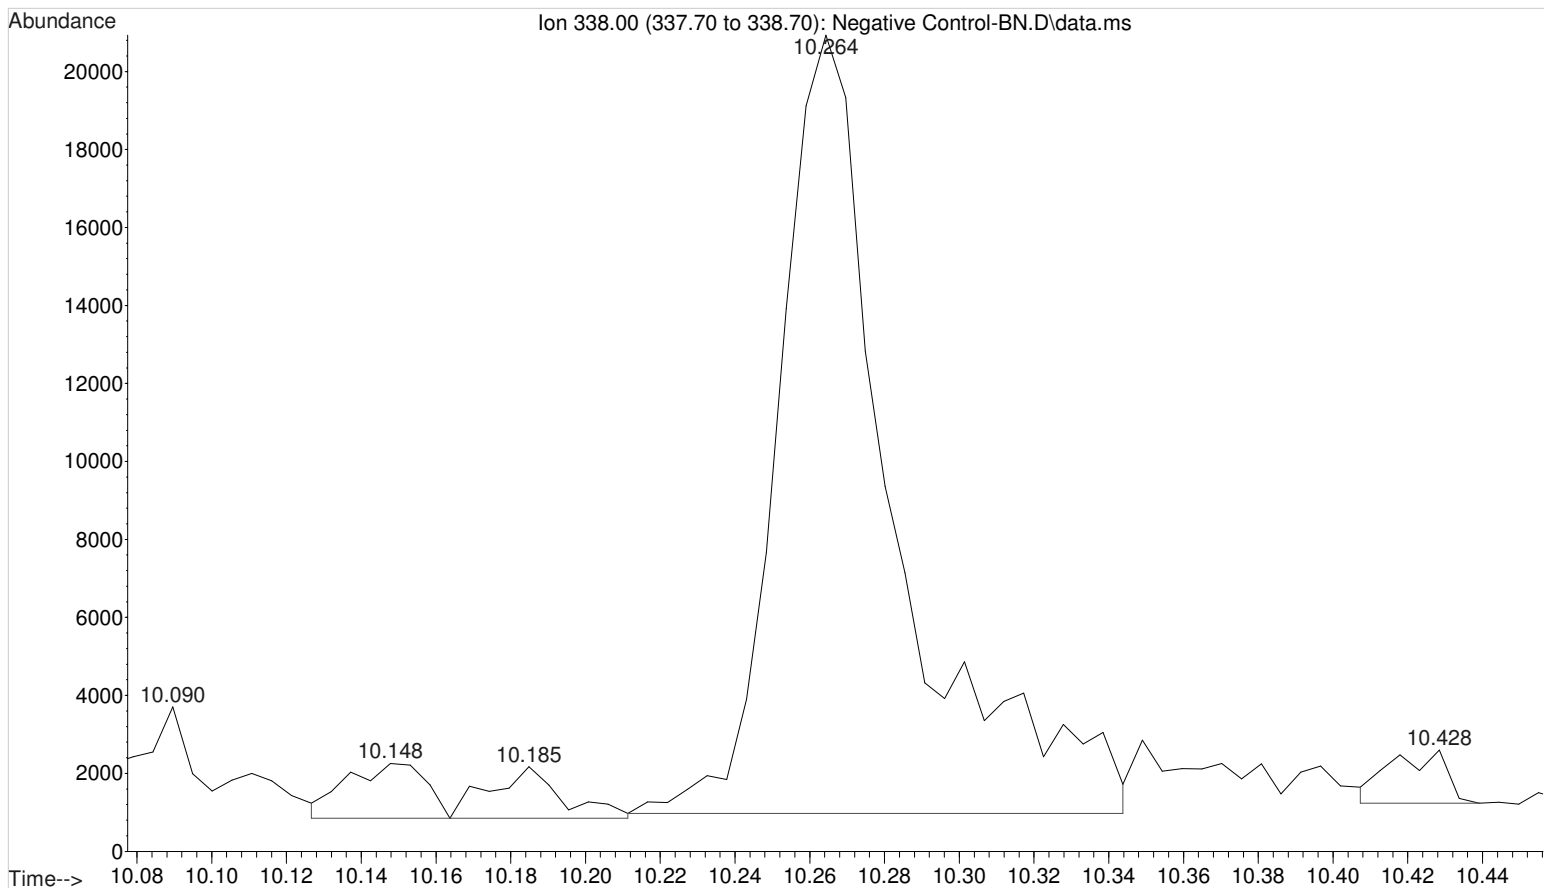



File :F:\11072016\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 07 Nov 2016 12:35 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

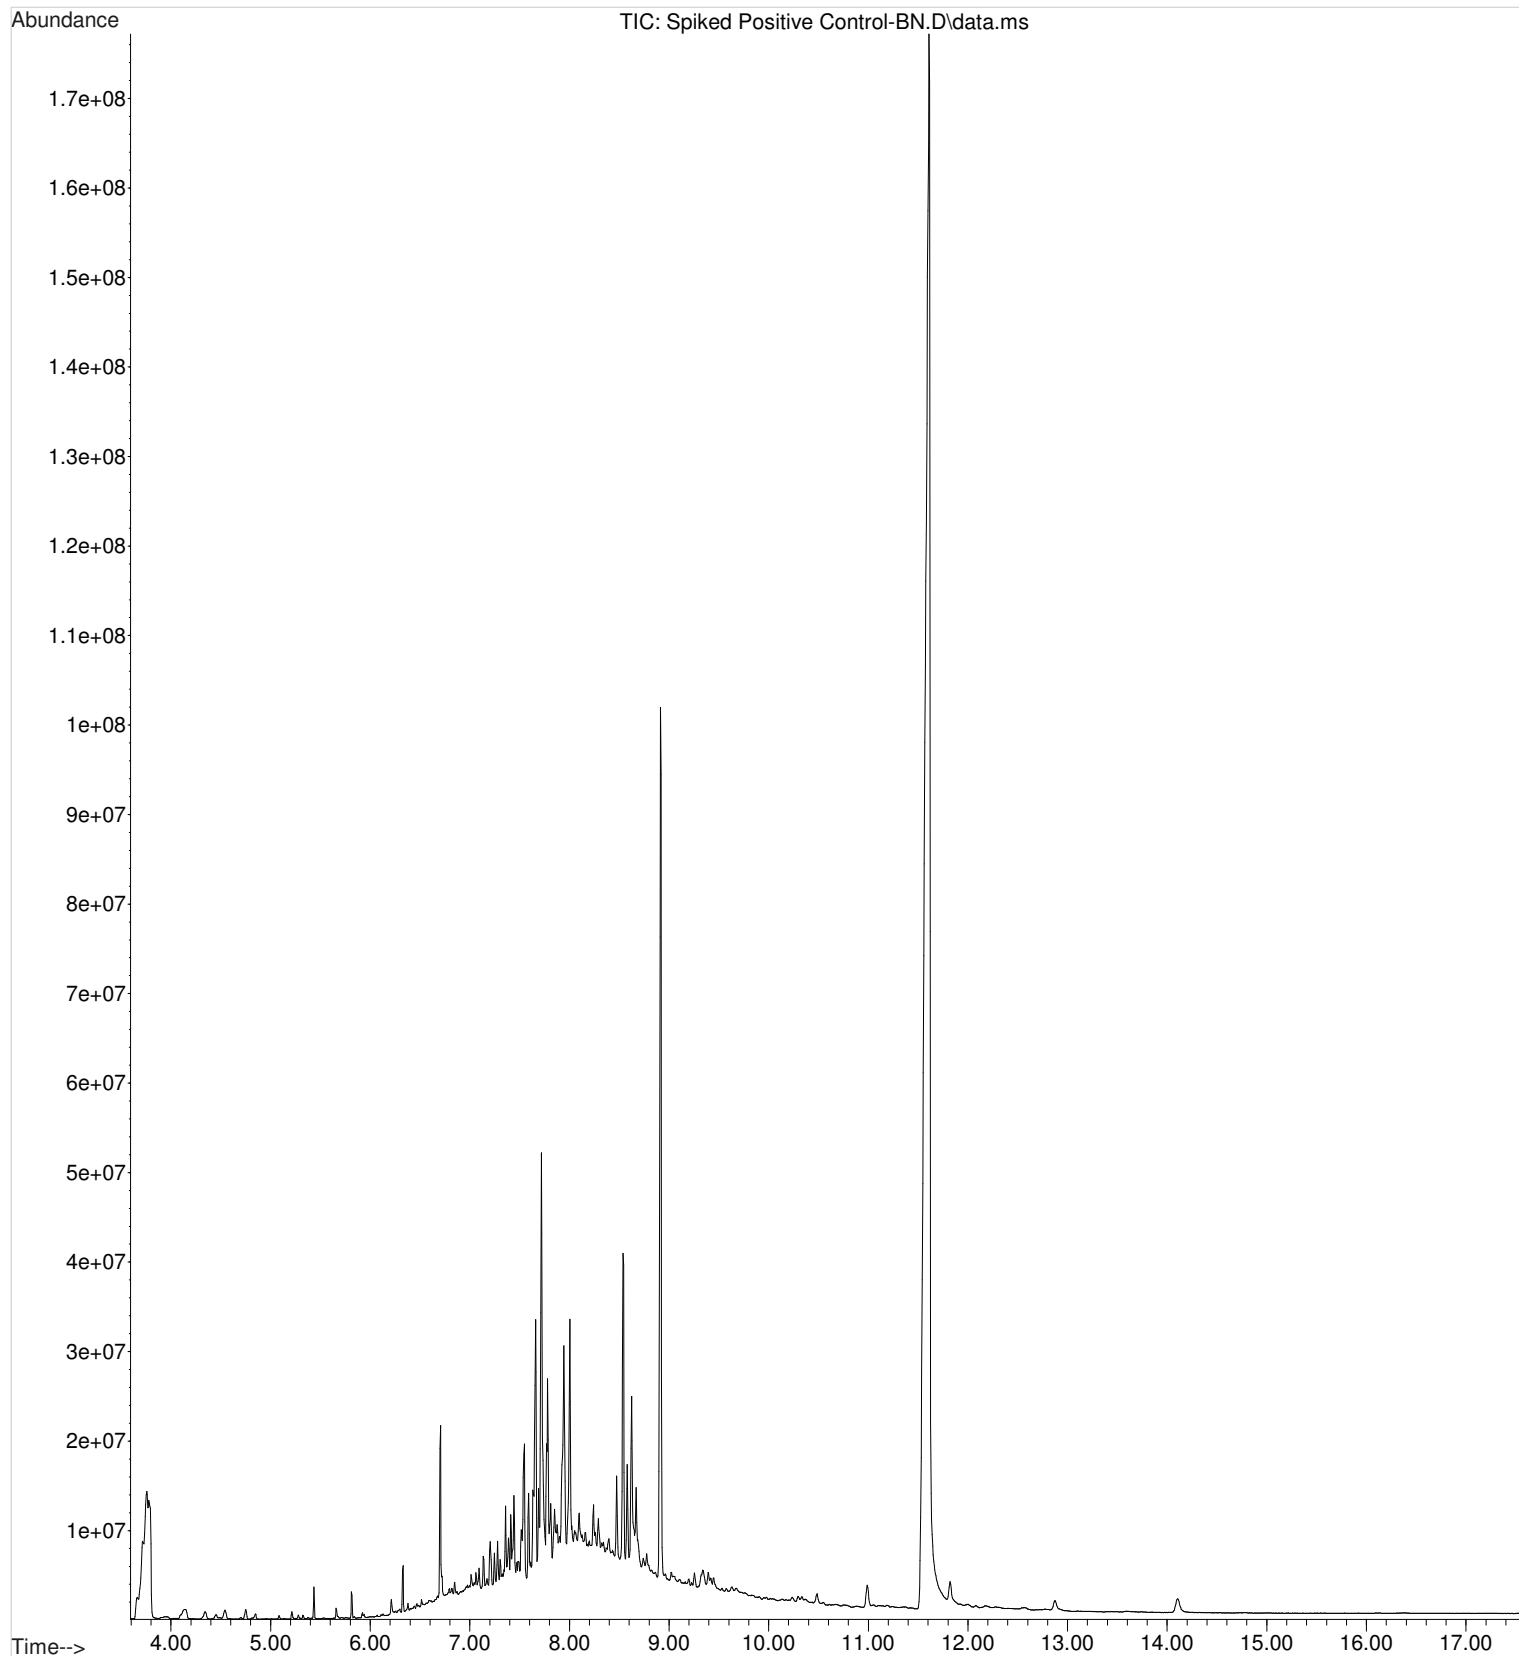



File : F:\11072016\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 07 Nov 2016 12:35 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

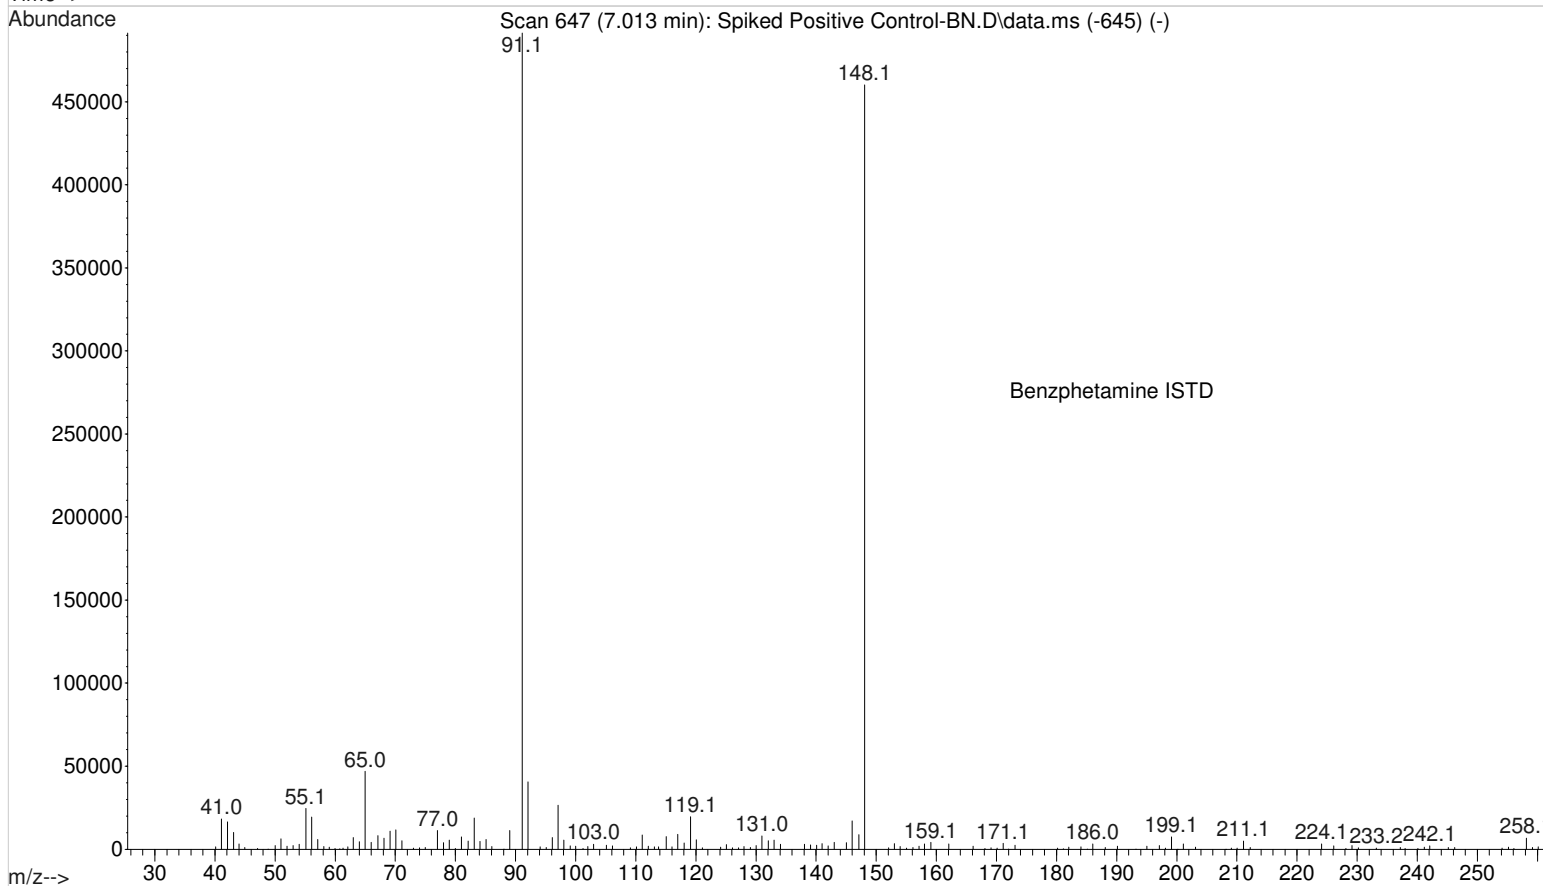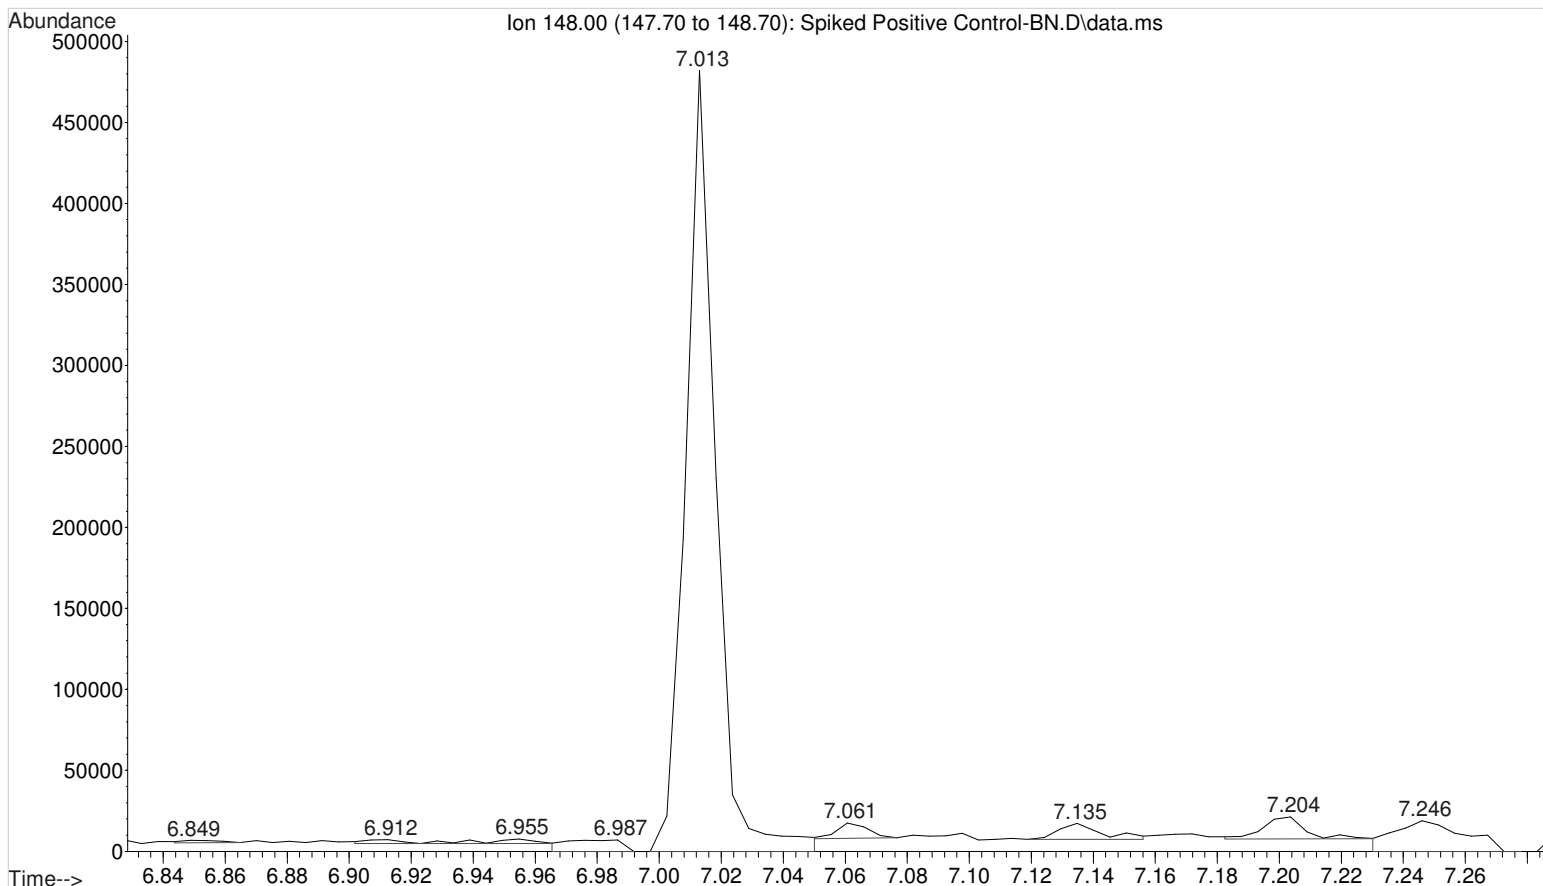



File : F:\11072016\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 07 Nov 2016 12:35 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

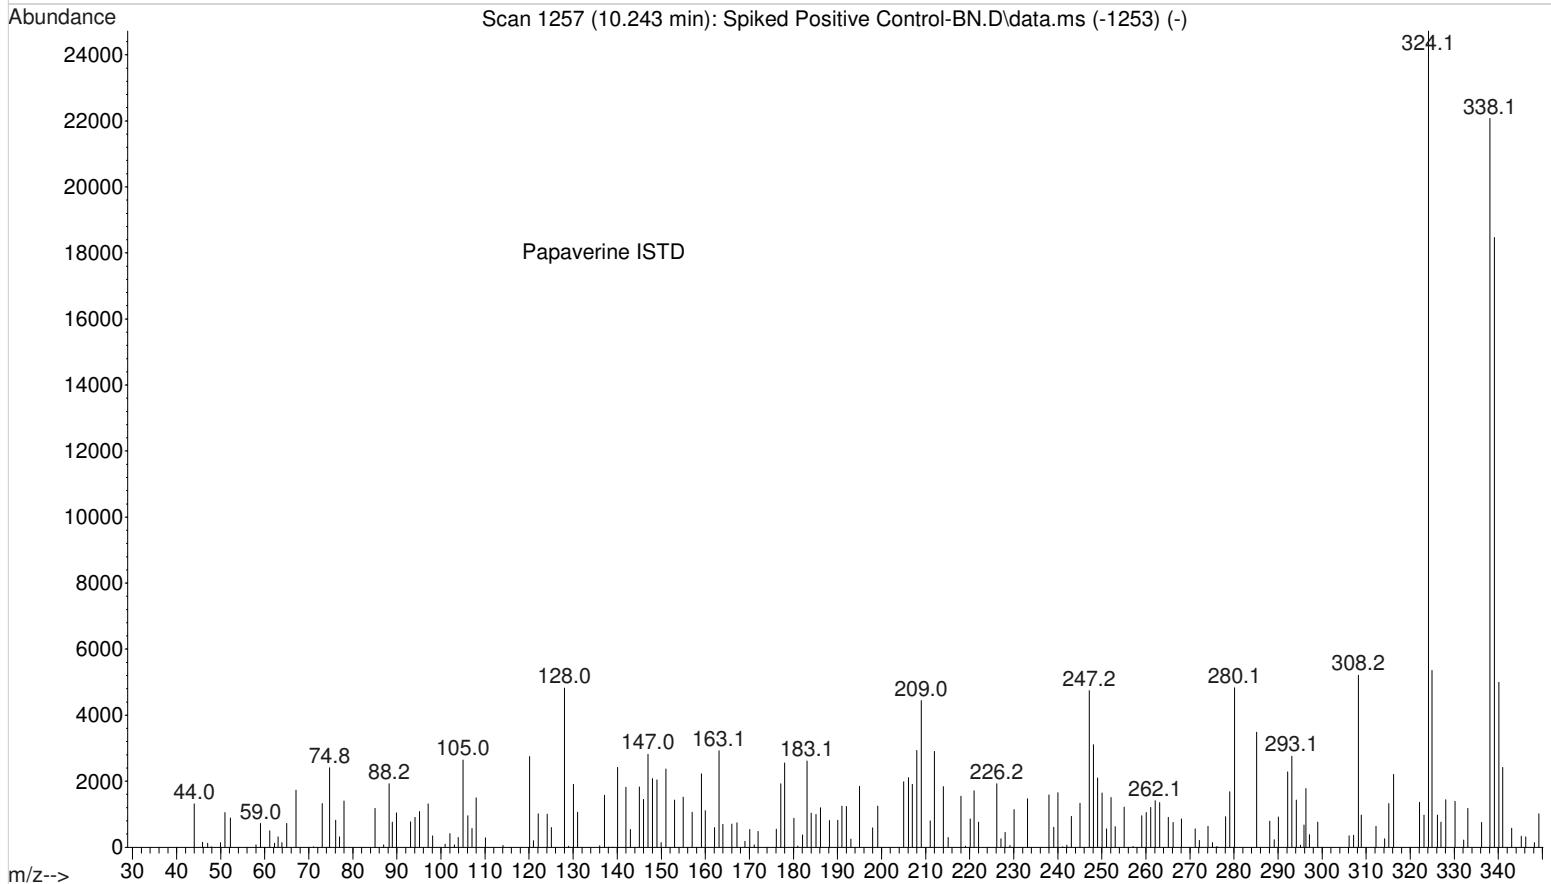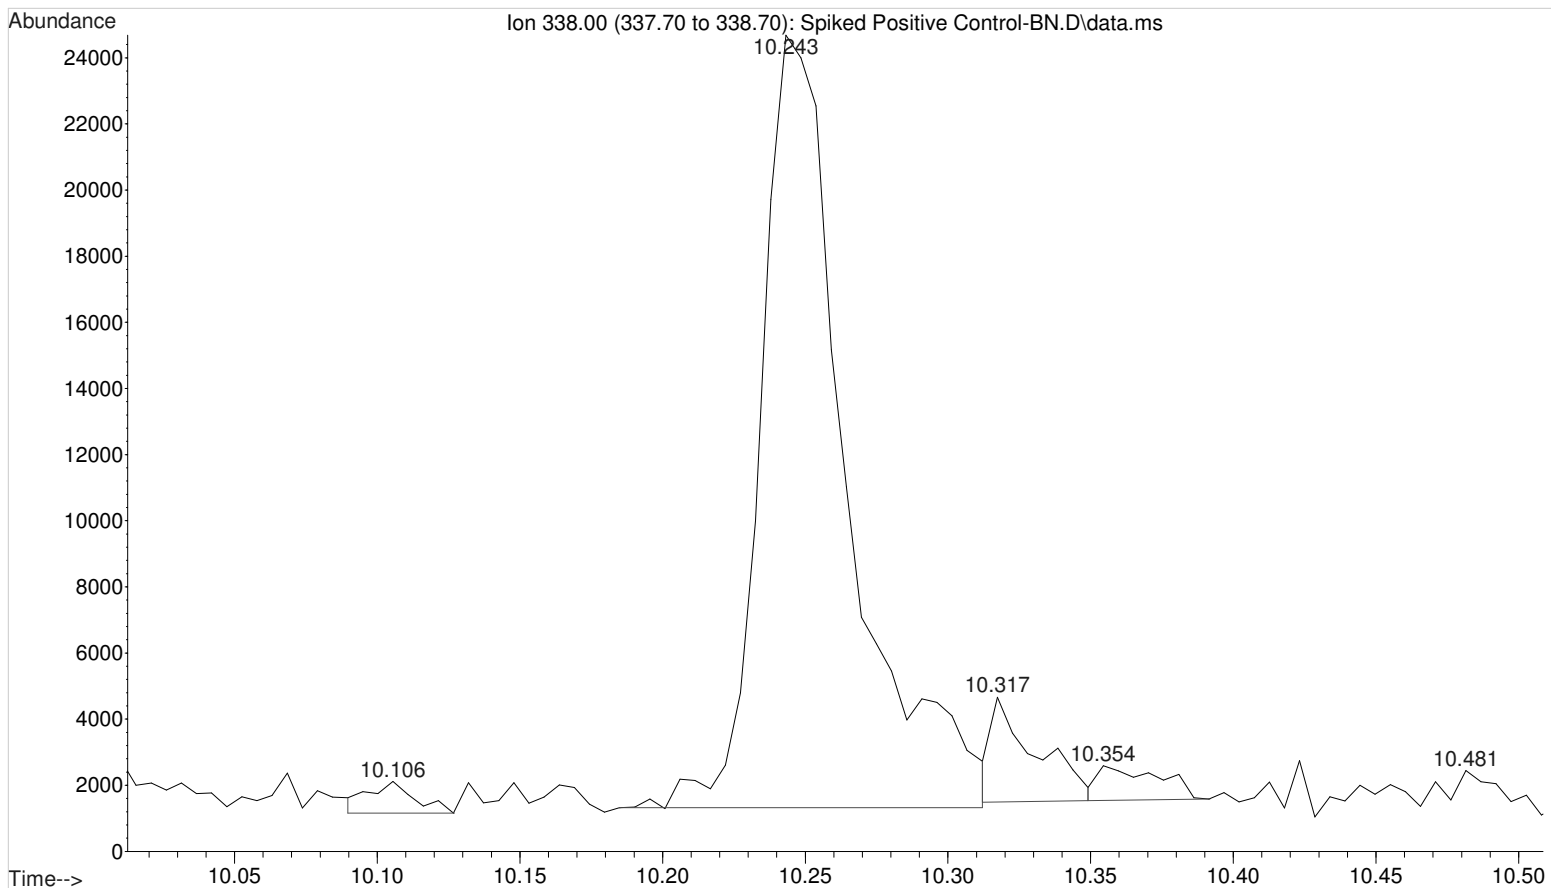



File : F:\11072016\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 07 Nov 2016 12:35 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name : Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

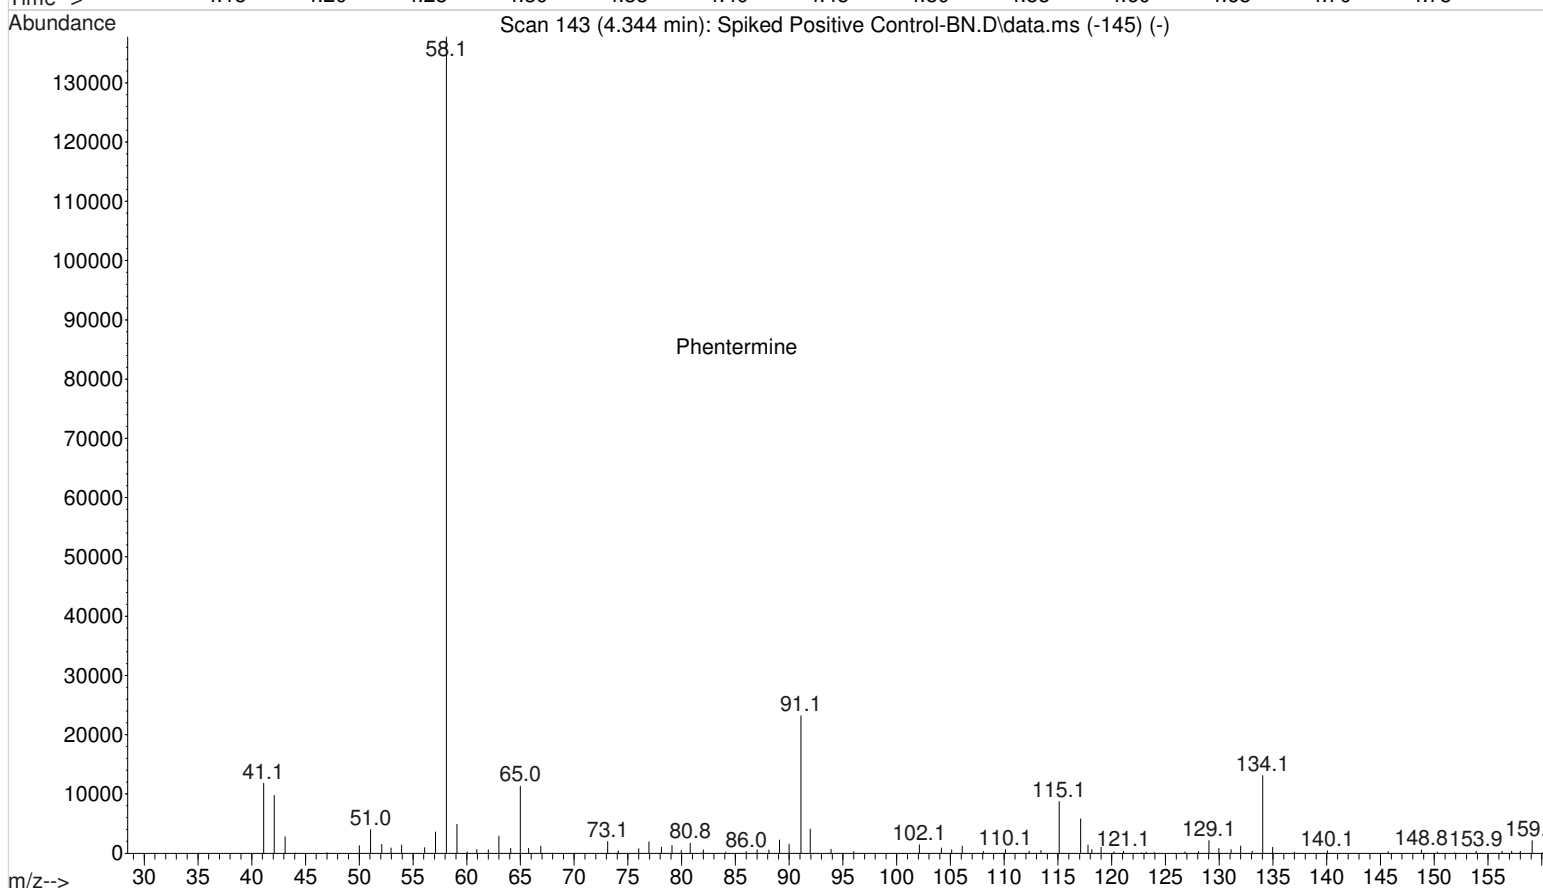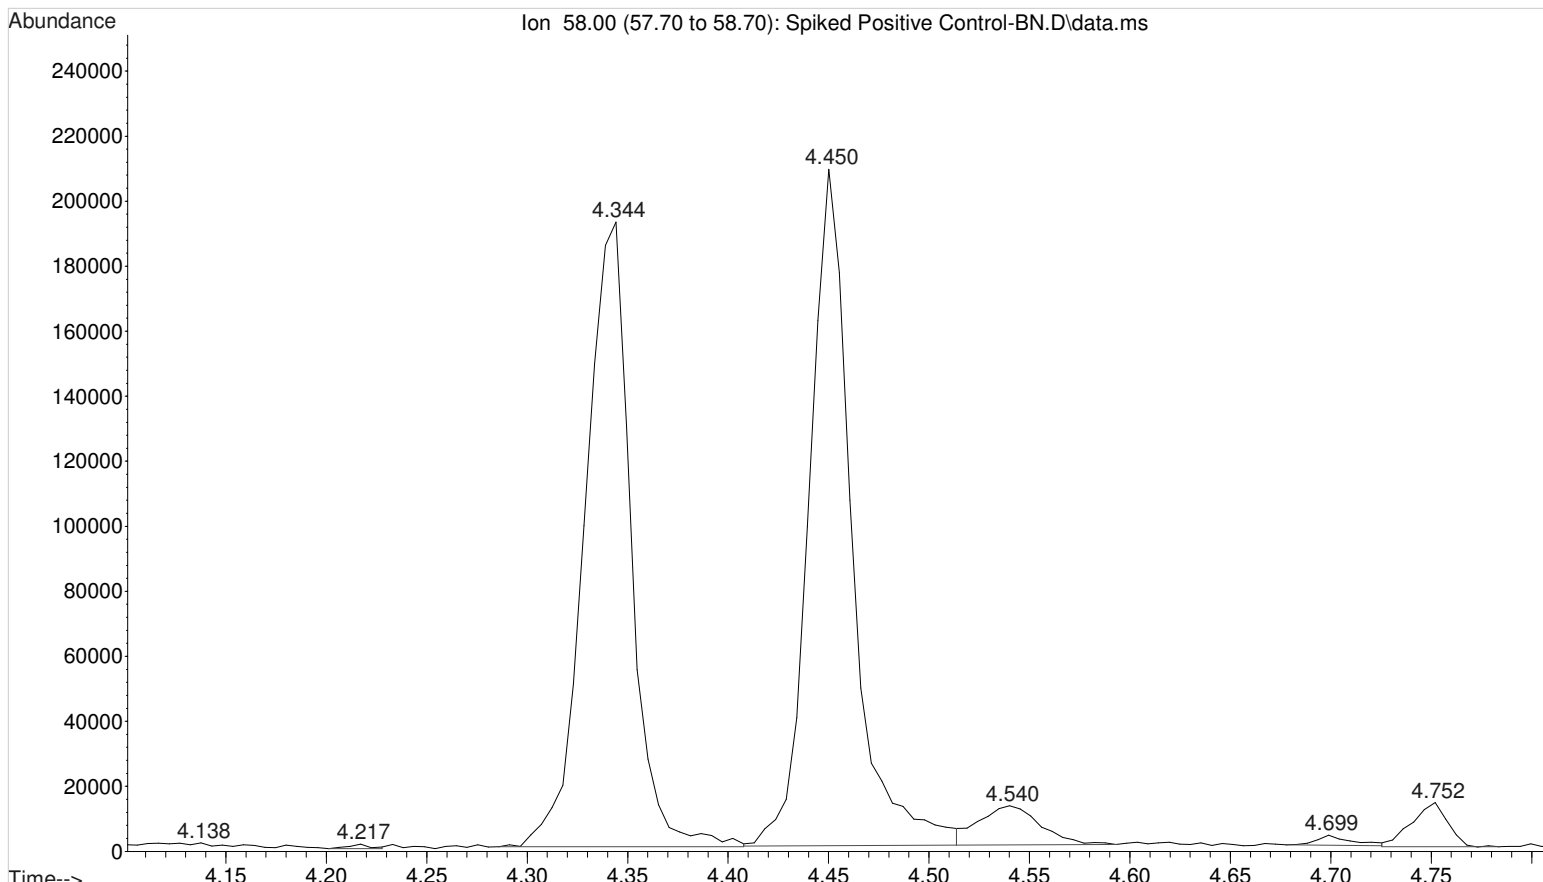



File : F:\11072016\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 07 Nov 2016 12:35 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name : Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

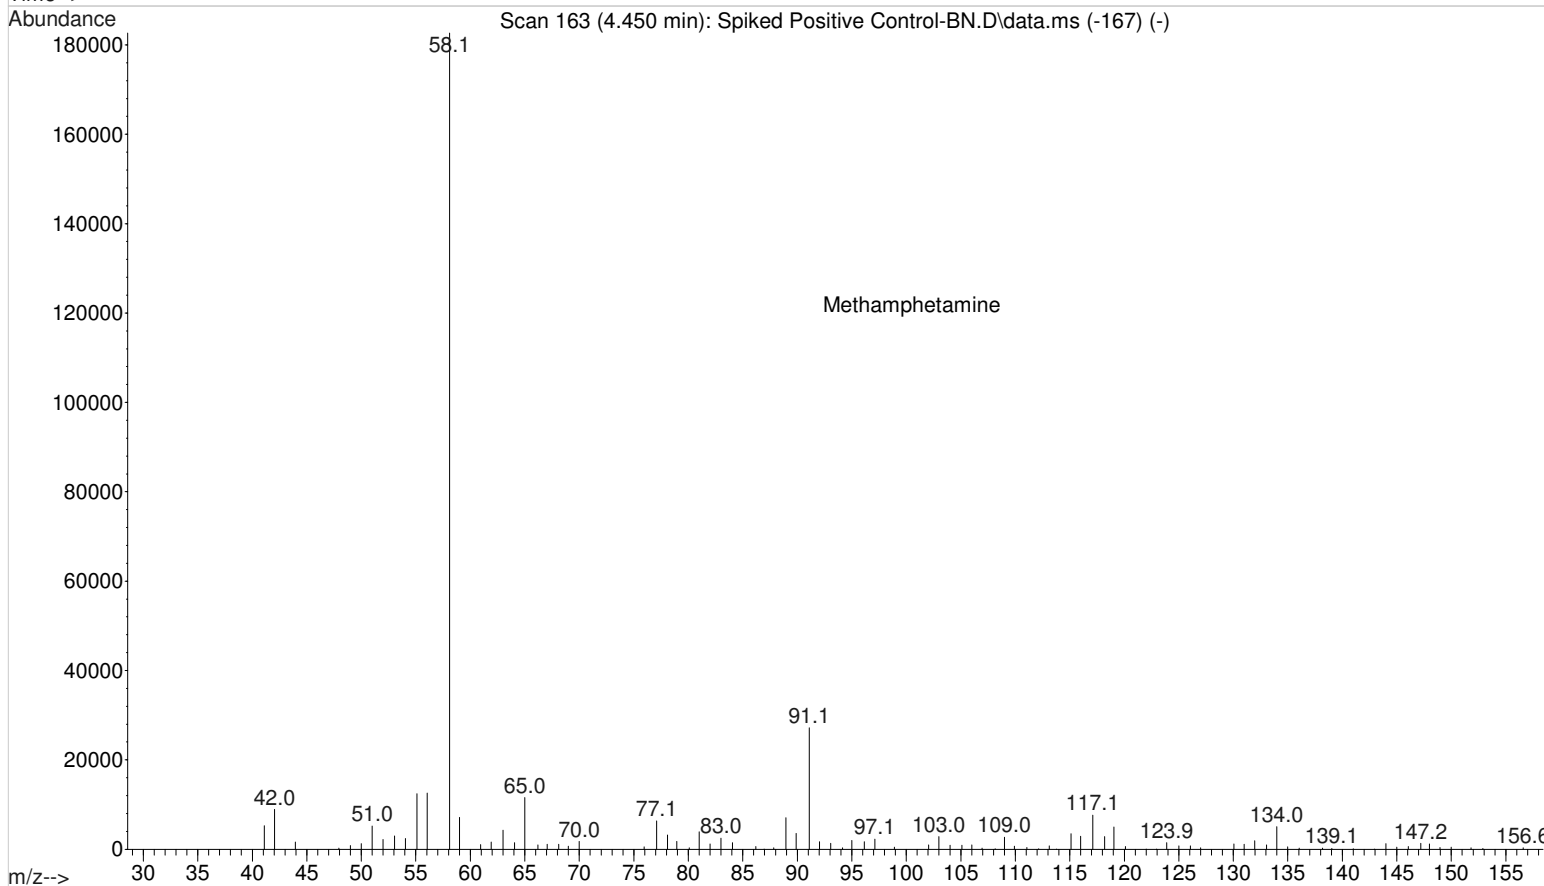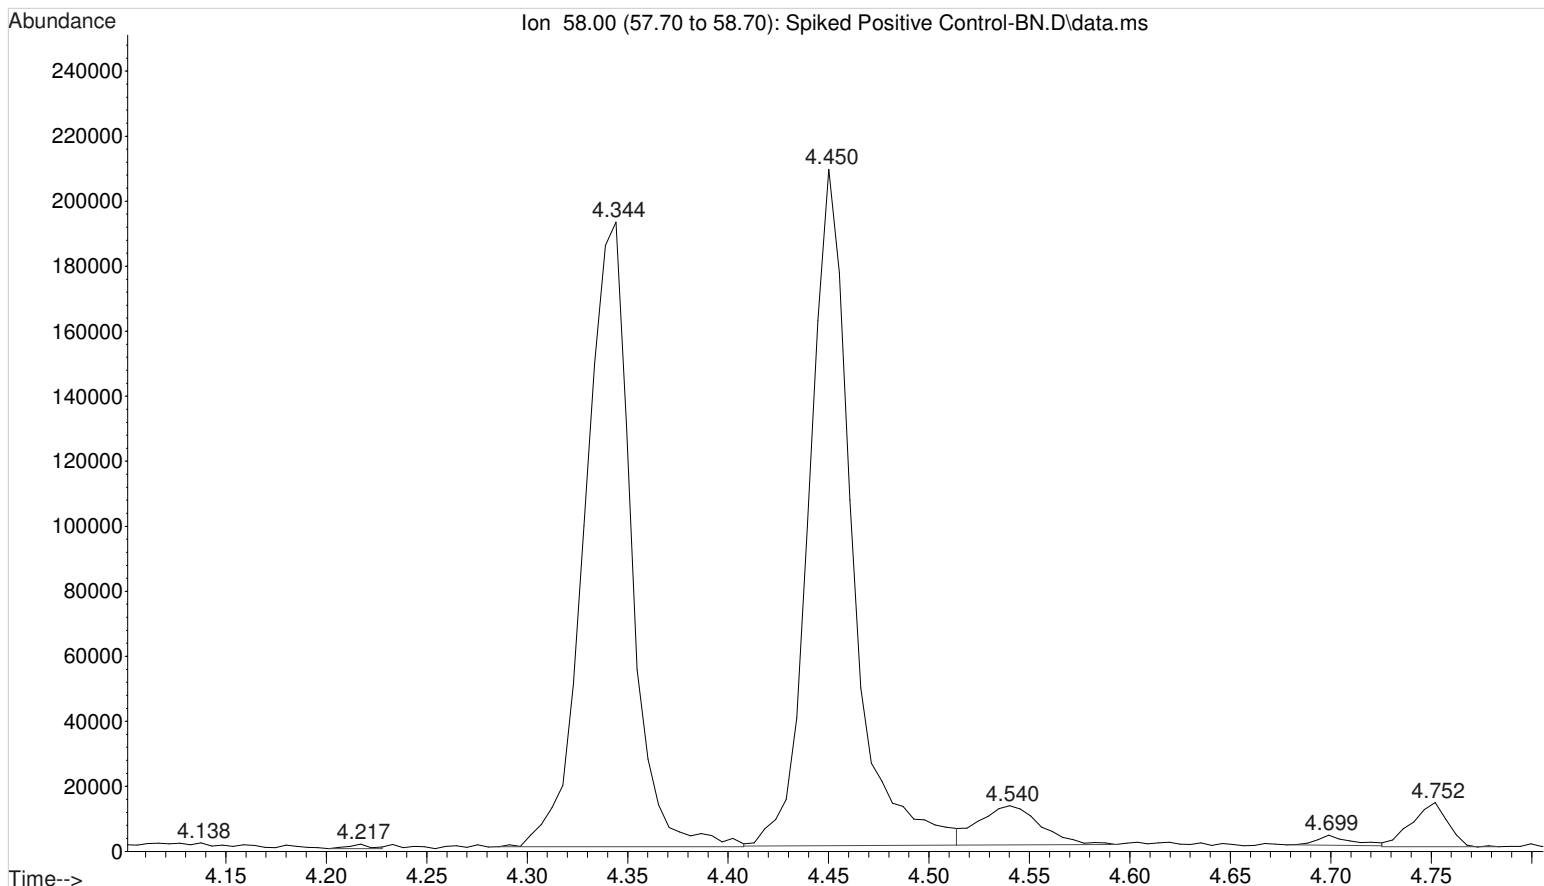



File : F:\11072016\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 07 Nov 2016 12:35 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

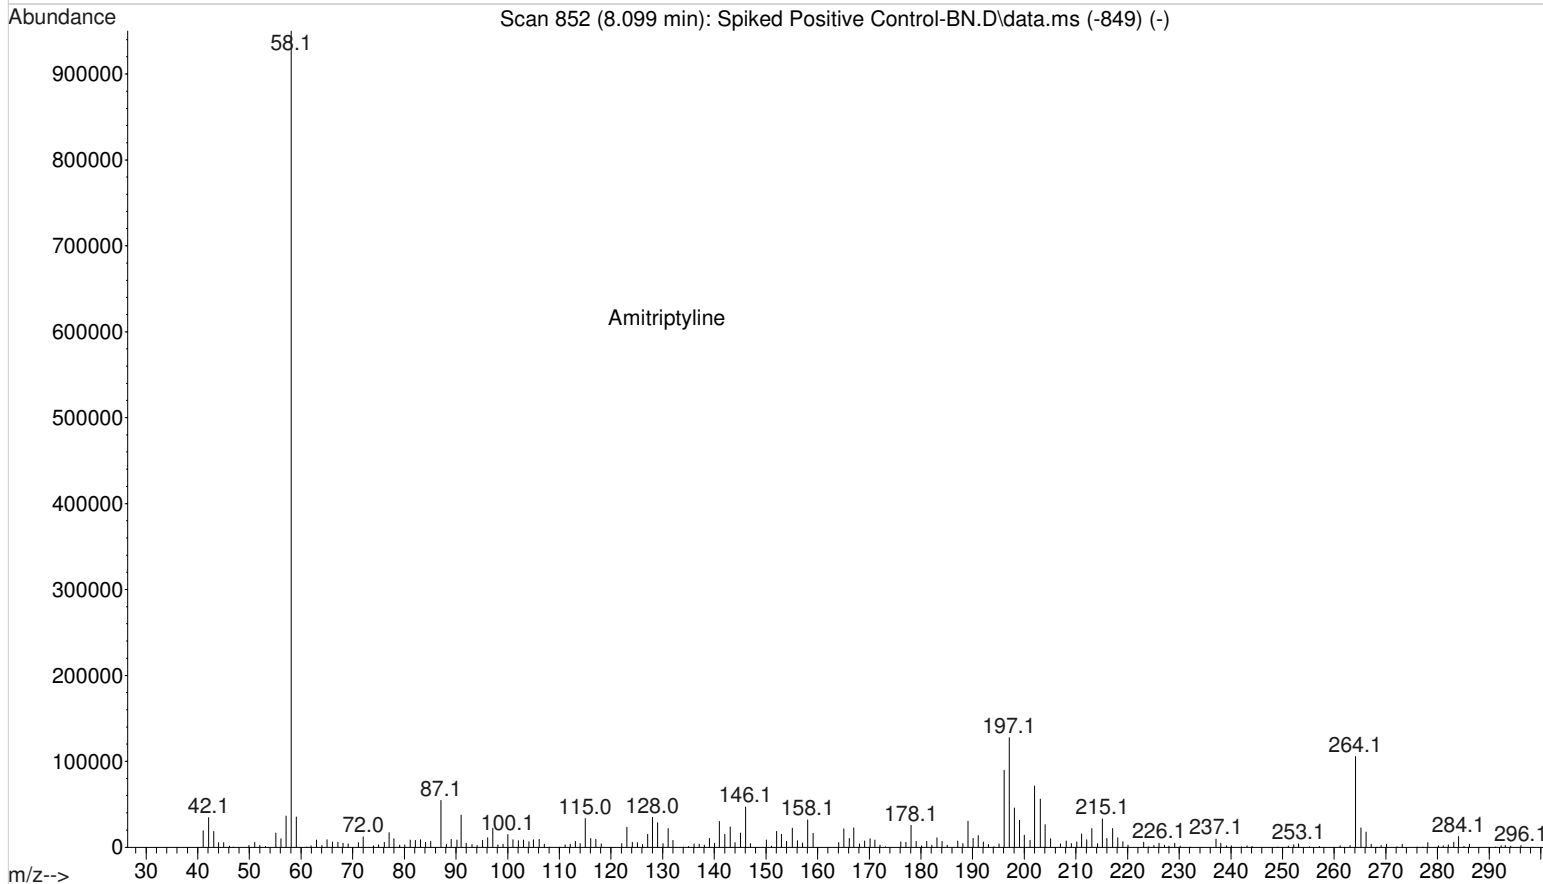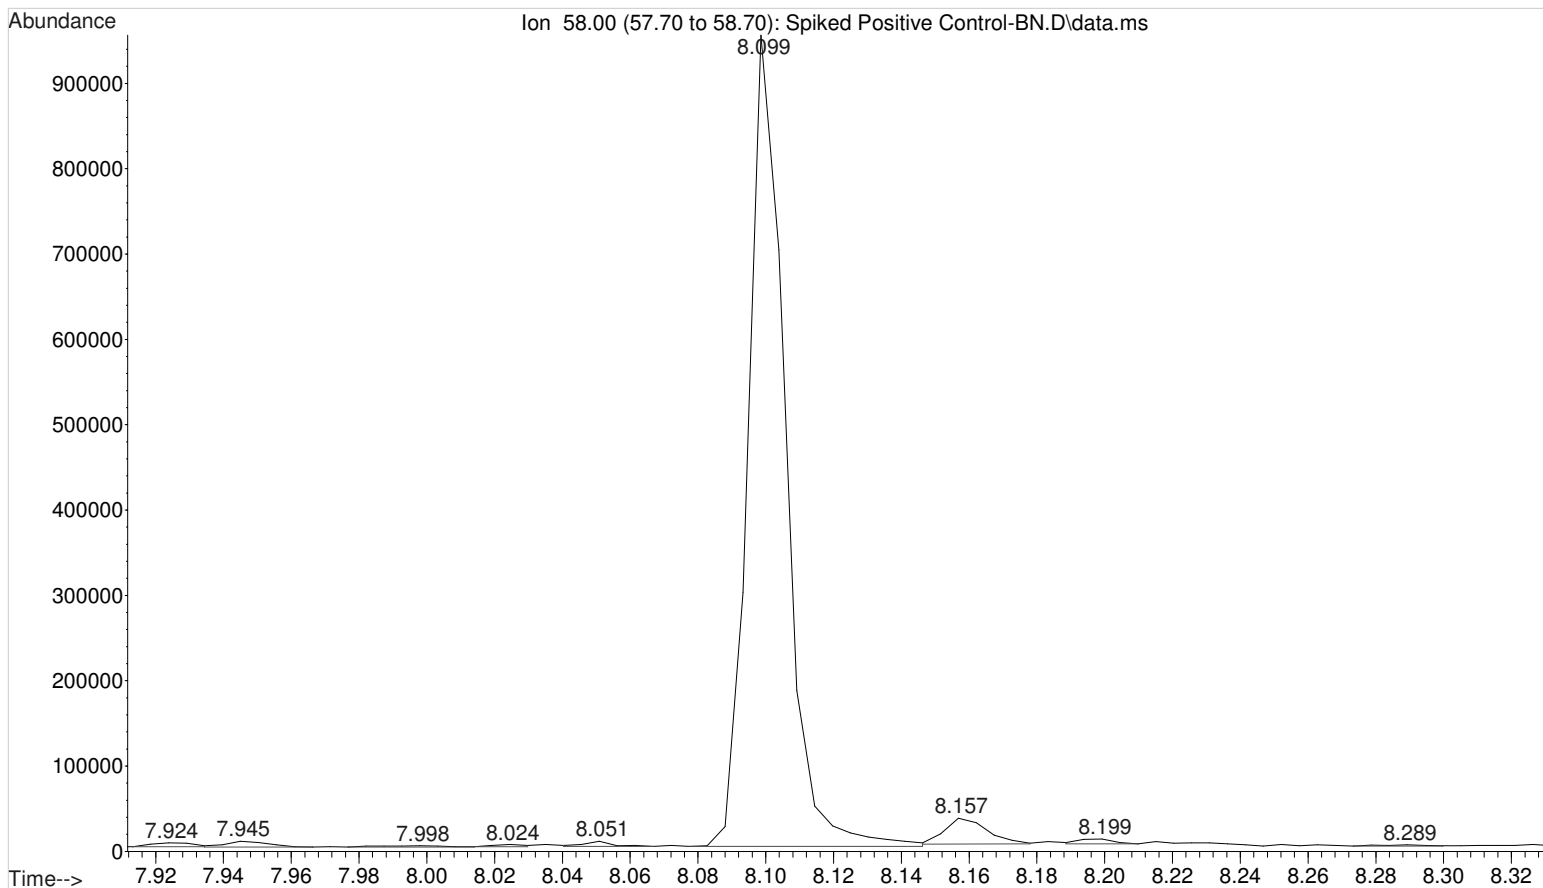

File : F:\11072016\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 07 Nov 2016 12:35 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name : Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

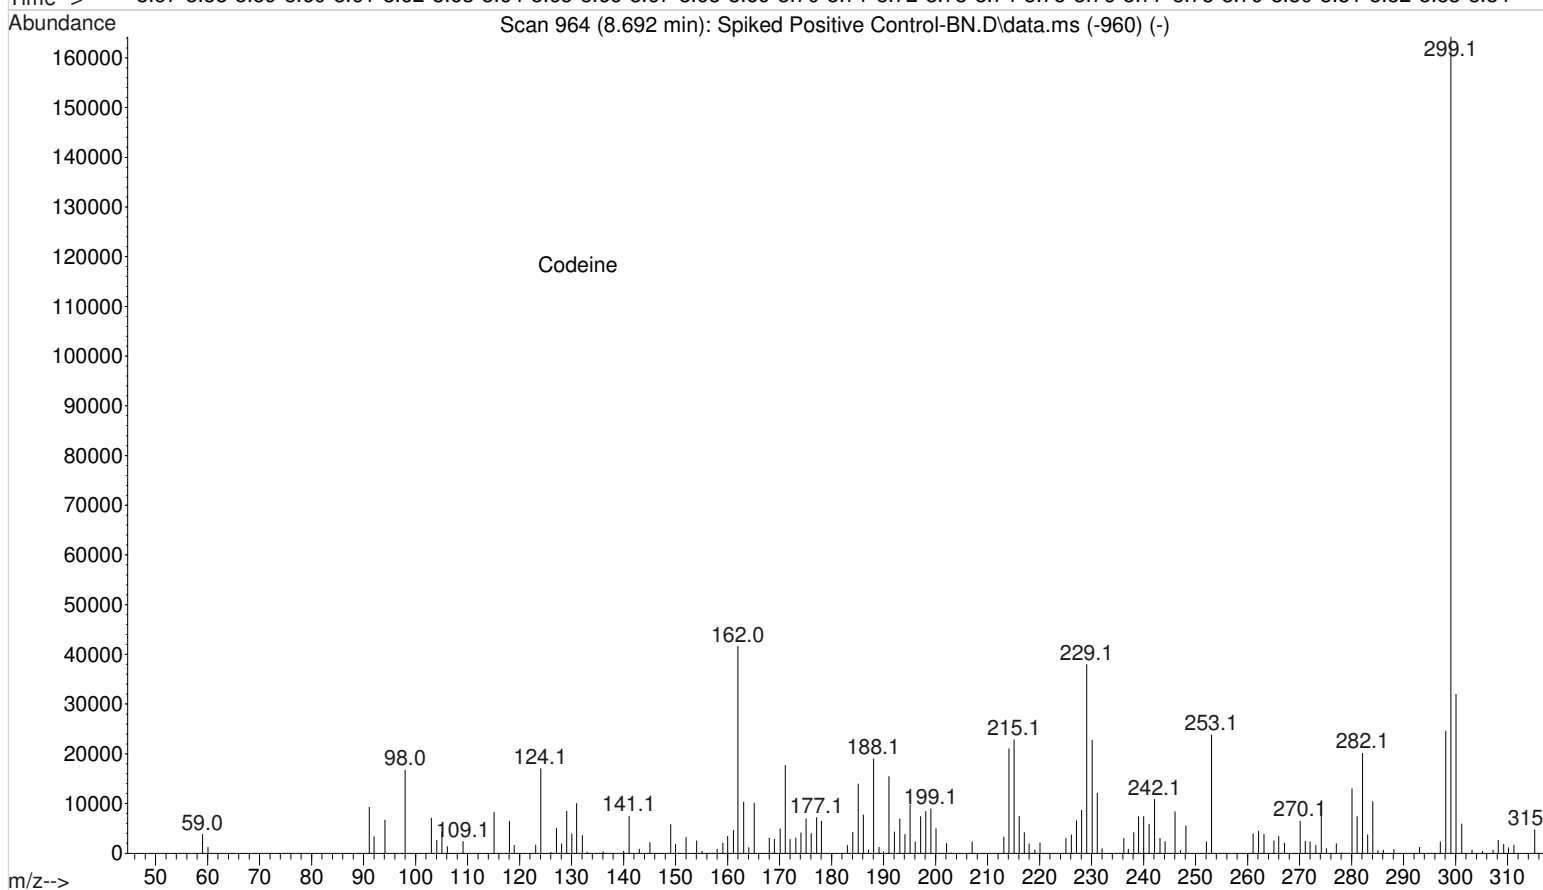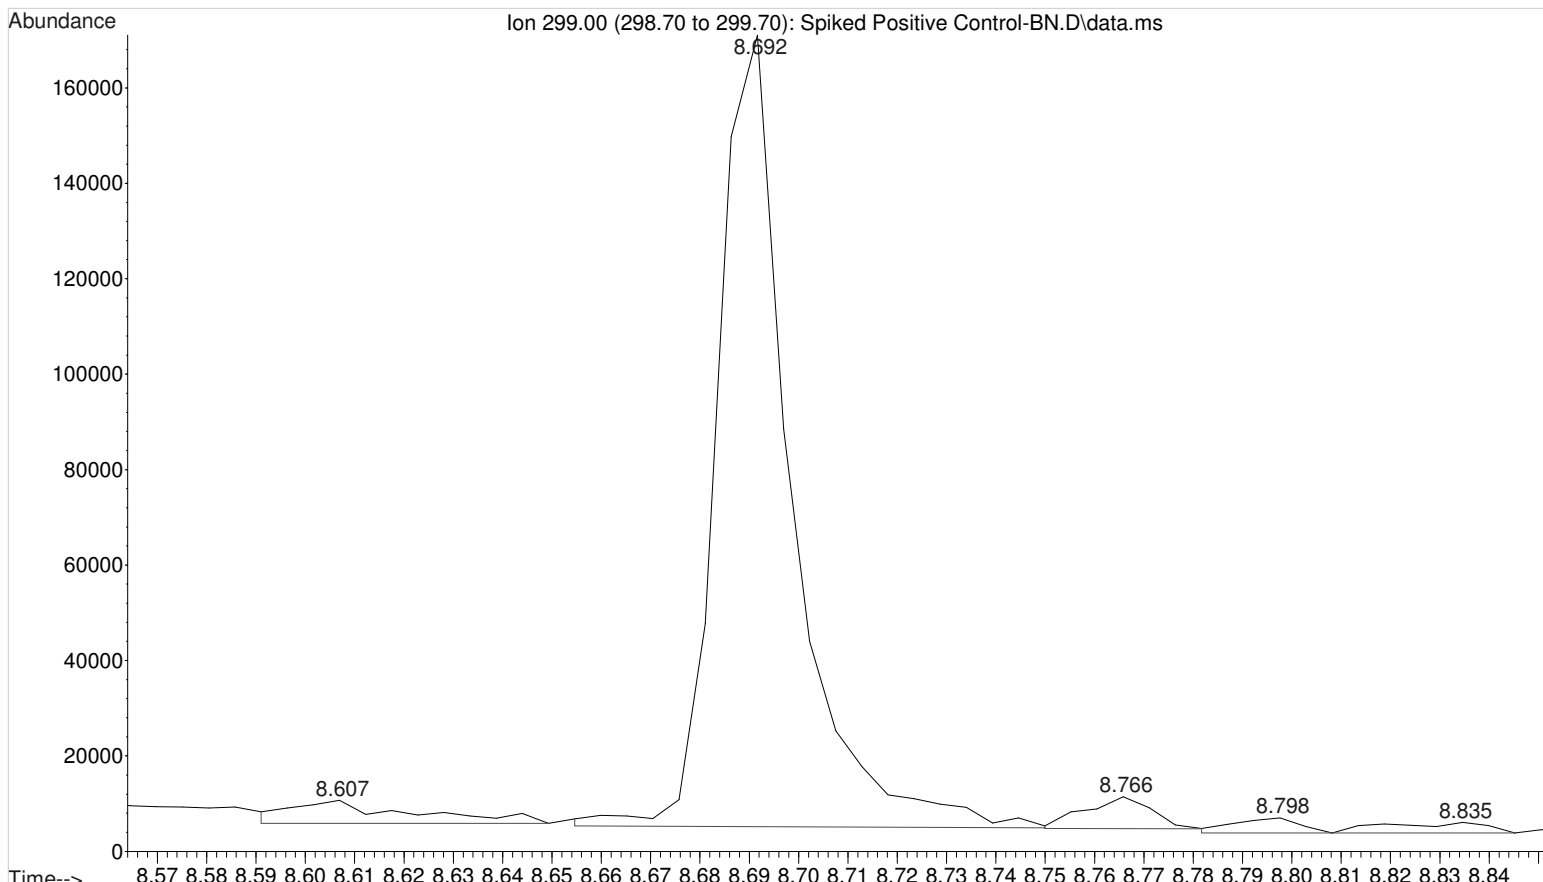


File : F:\11072016\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 07 Nov 2016 12:35 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name : Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

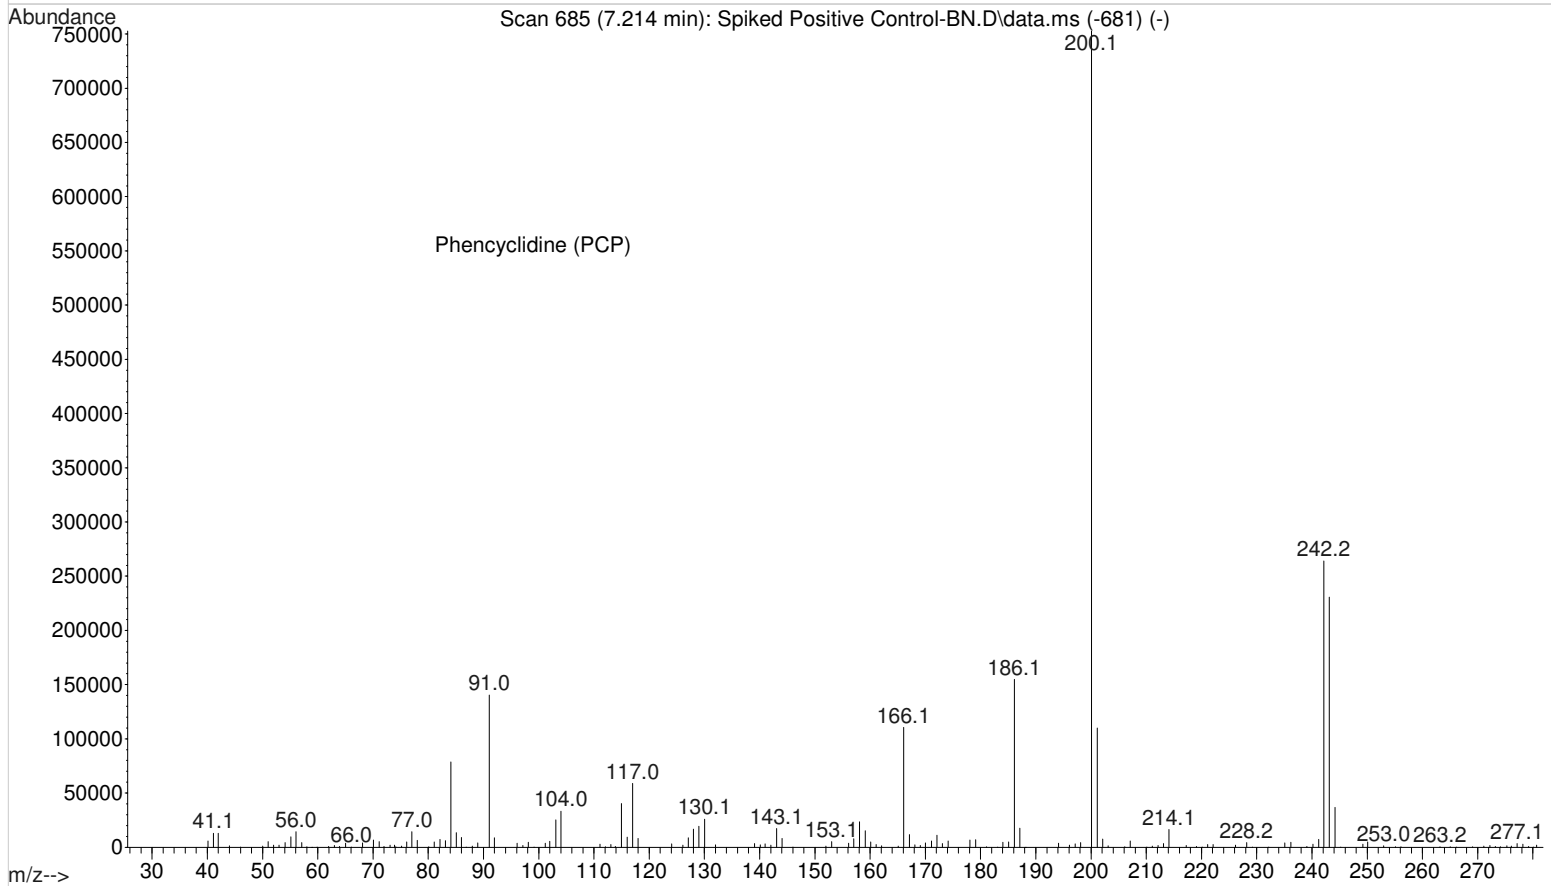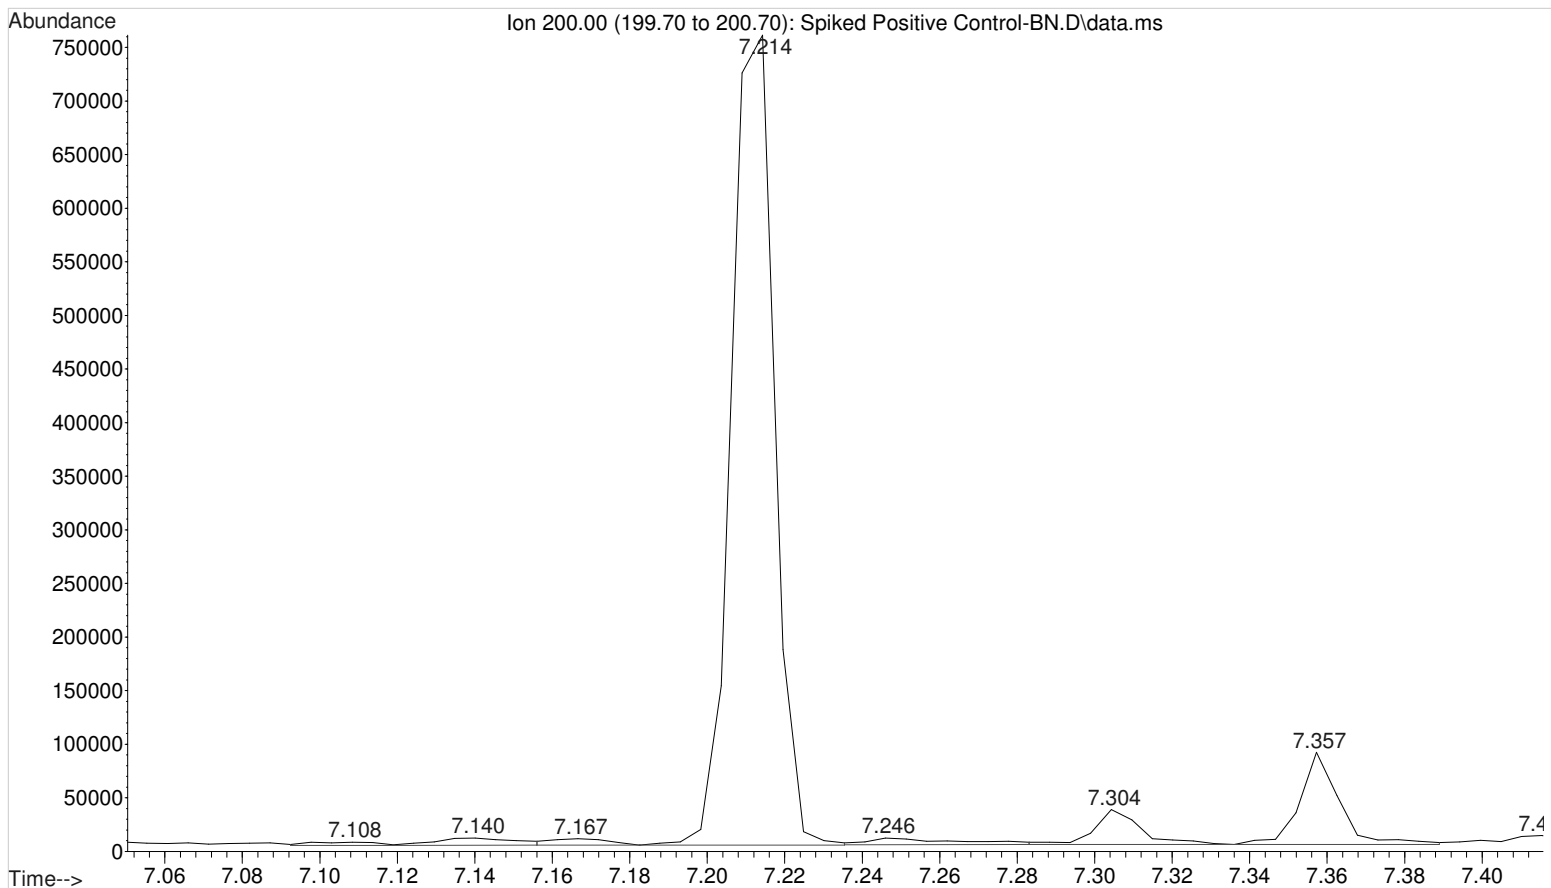


ISP


File :F:\11072016\Prerun Solvent Blankr.D
Operator : ISP\datastor
Acquired : 07 Nov 2016 13:20 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Pre-run Solvent Blank
Misc Info : Chloroform
Vial Number: 100

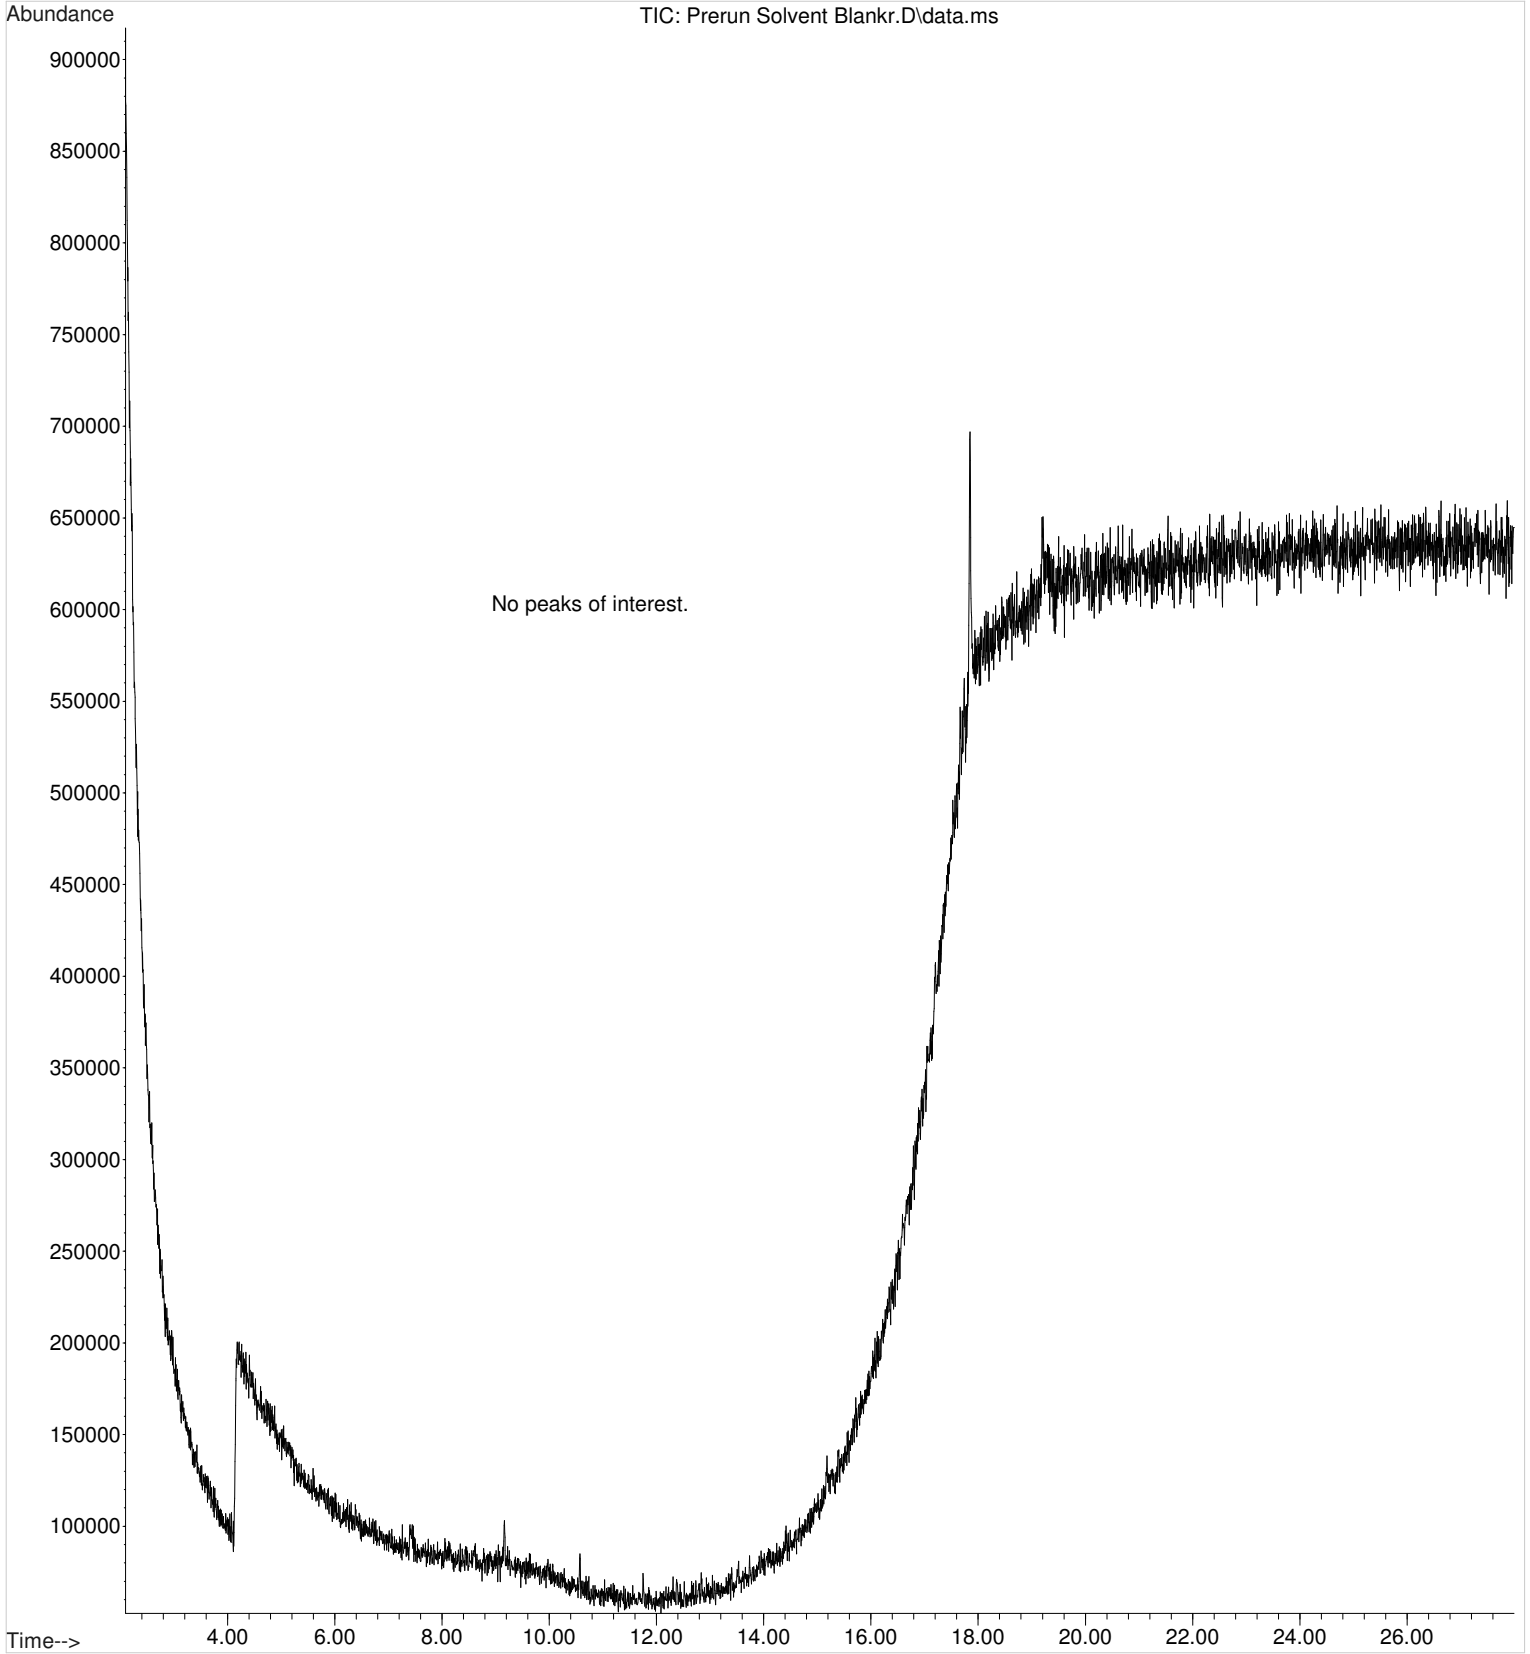



File :F:\11072016\prbLK2r.D
Operator : ISP\datastor
Acquired : 07 Nov 2016 15:02 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Solvent Blank
Misc Info : Chloroform
Vial Number: 99

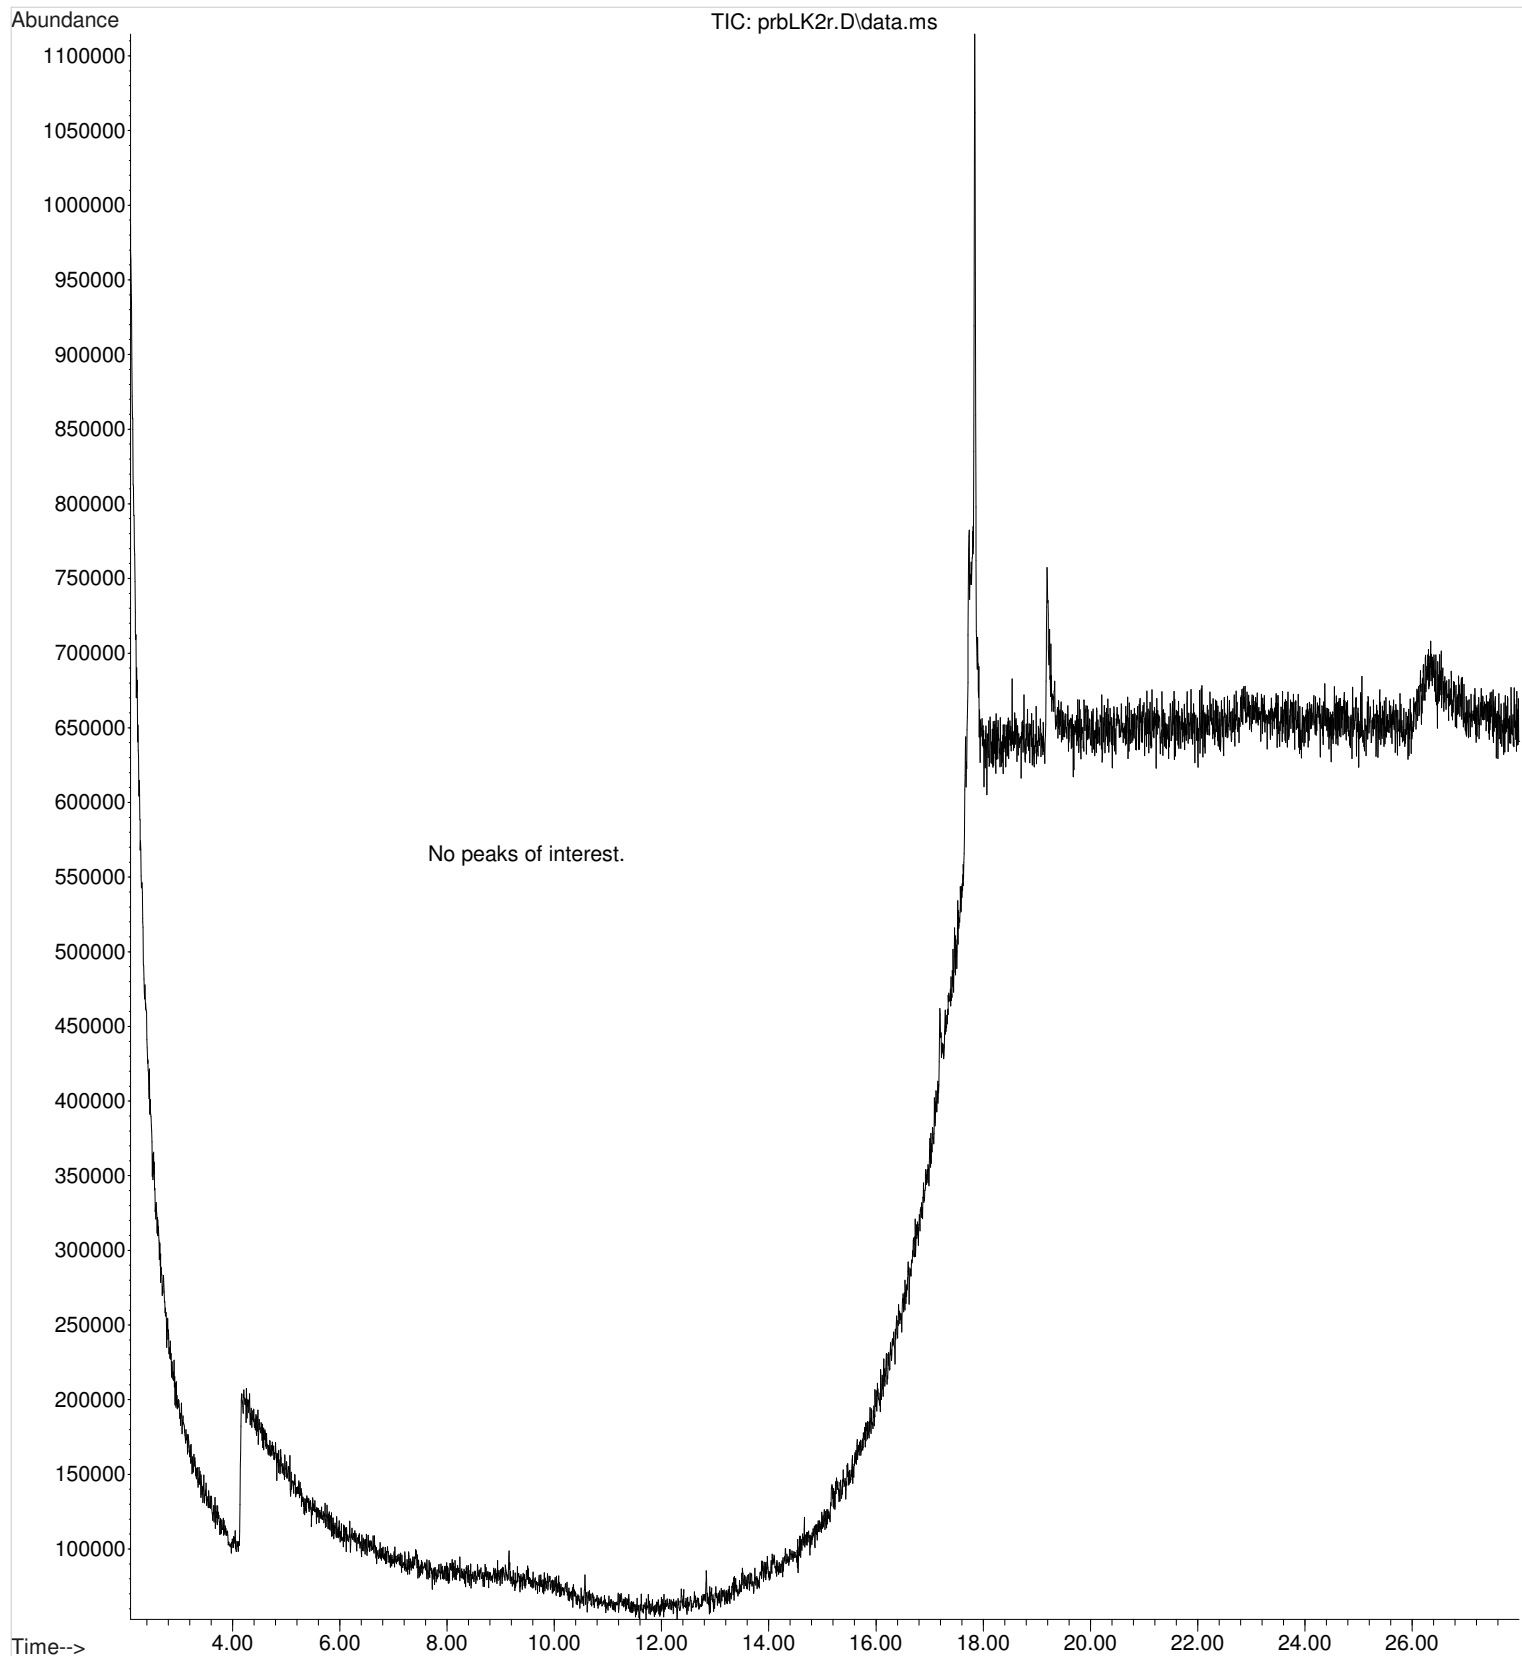



File :F:\11072016\Negative Control-BNr.D
Operator : ISP\datastor
Acquired : 07 Nov 2016 13:54 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B1013
Misc Info : Analytical Method 3.6.1
Vial Number: 1

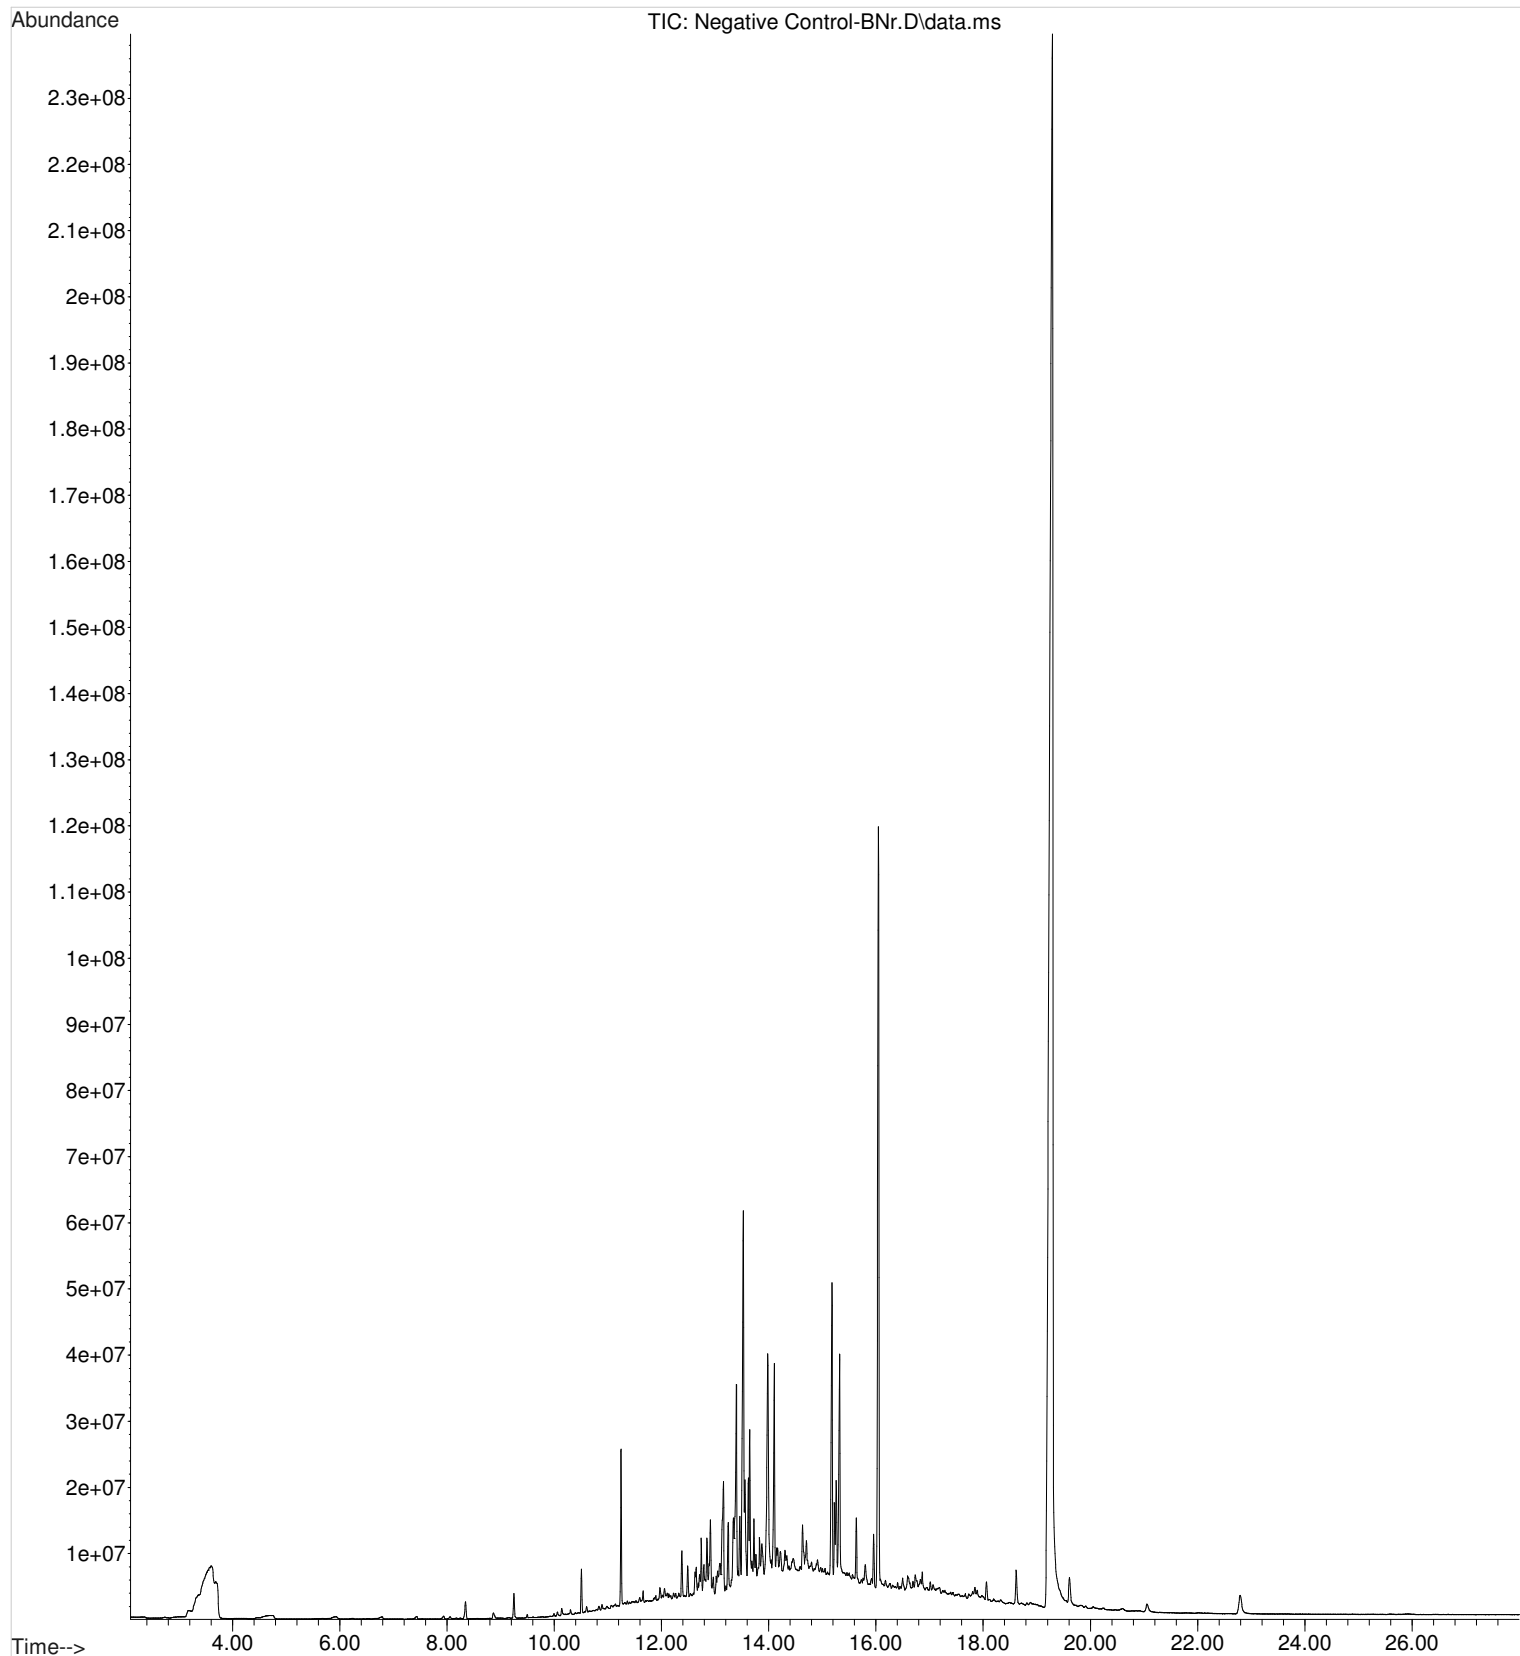

File : F:\11072016\Negative Control-BNr.D
Operator : ISP\datastor
Acquired : 07 Nov 2016 13:54 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name : Negative Control - Utak Lot B1013
Misc Info : Analytical Method 3.6.1
Vial Number: 1

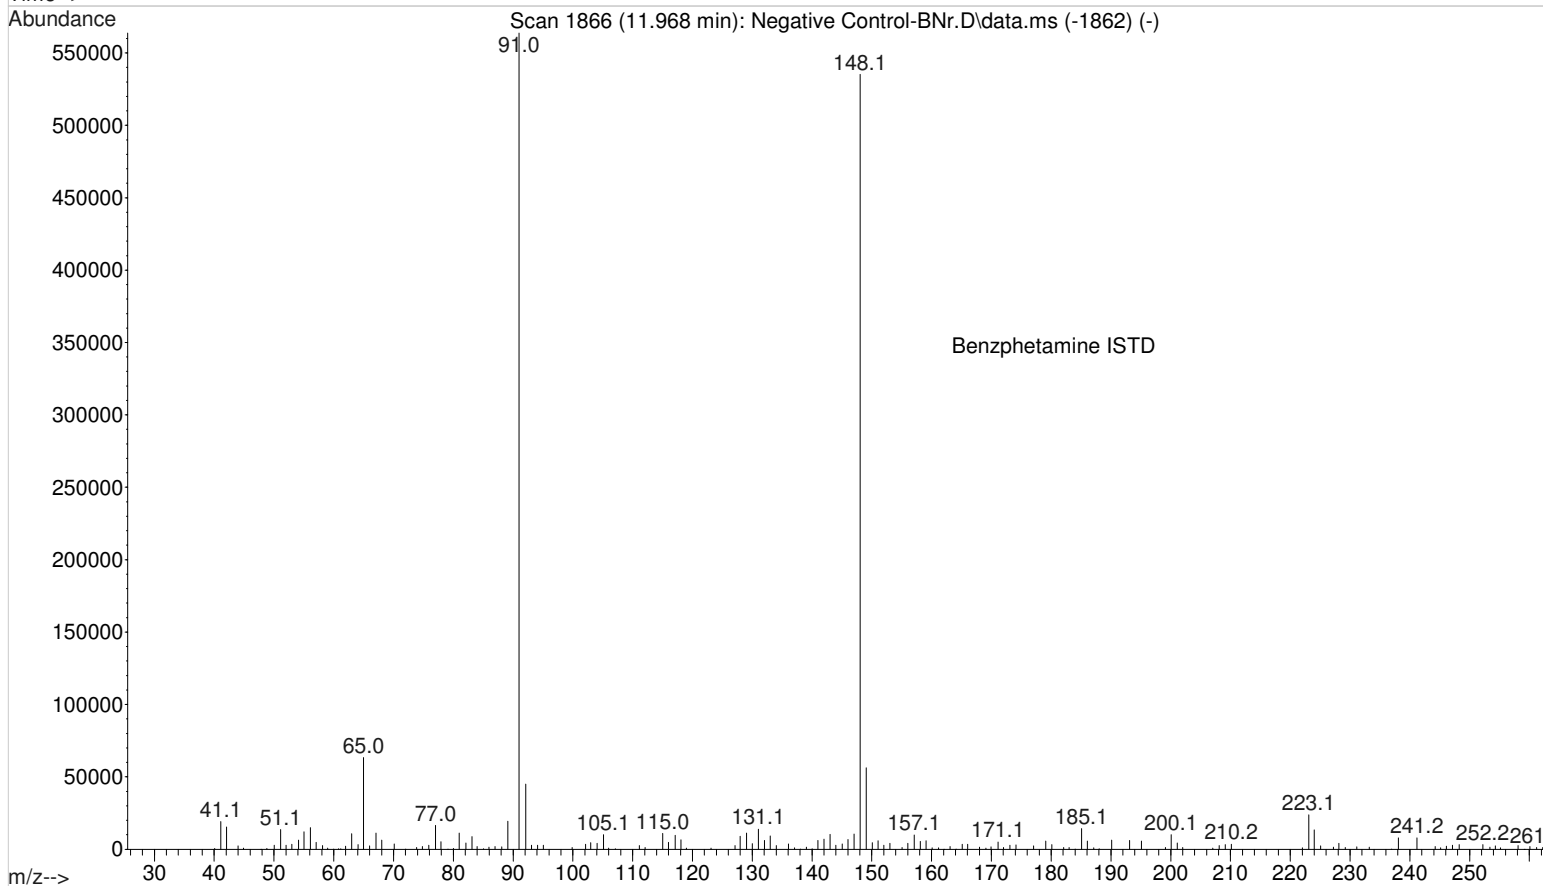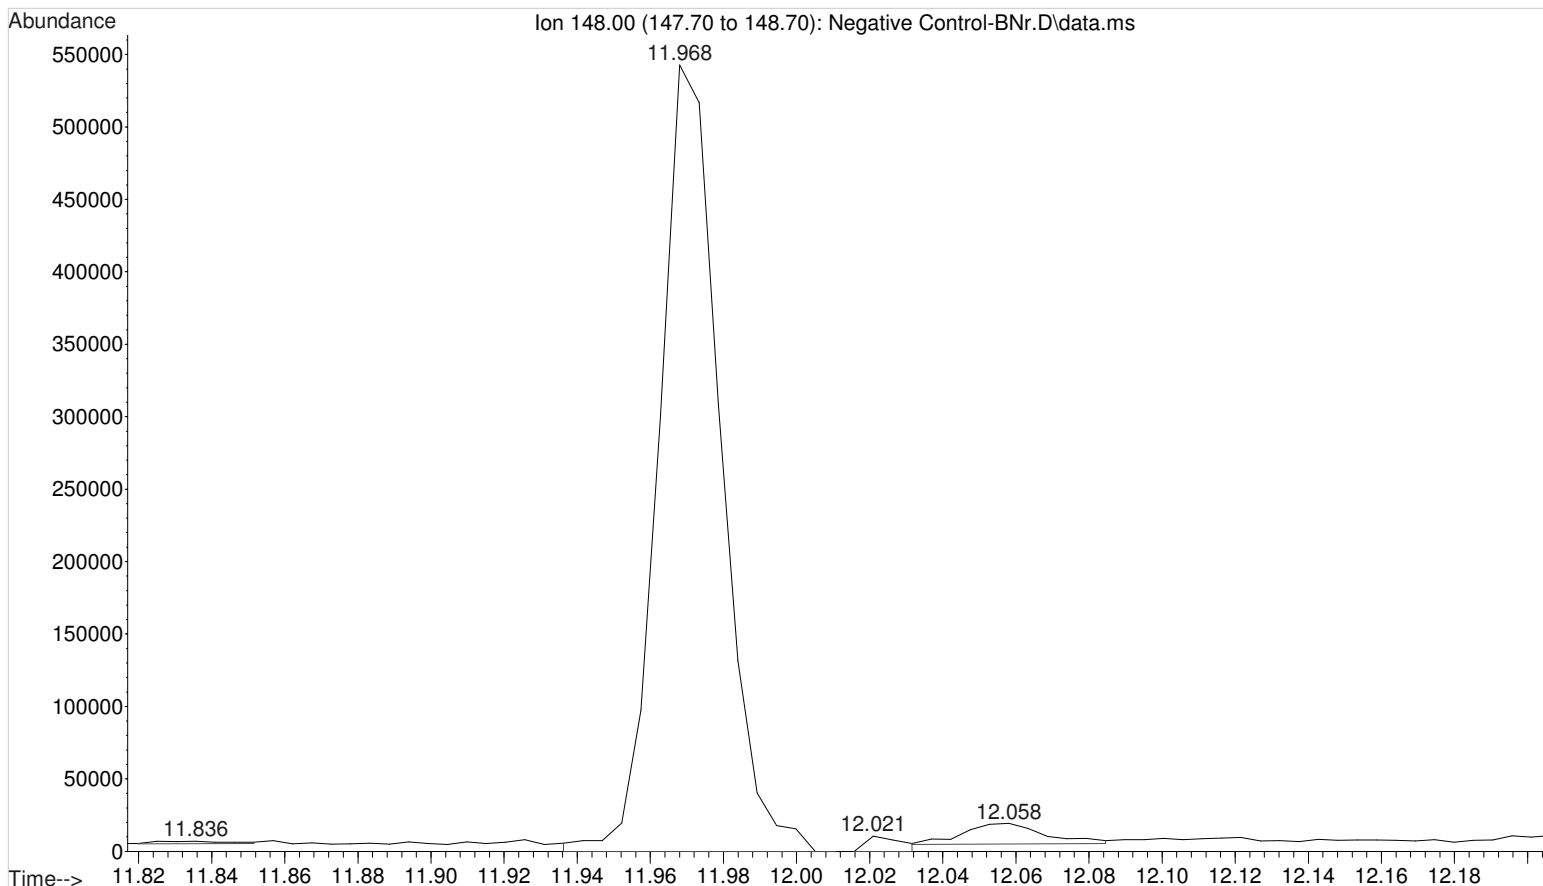


File : F:\11072016\Negative Control-BNr.D
Operator : ISP\datastor
Acquired : 07 Nov 2016 13:54 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name : Negative Control - Utak Lot B1013
Misc Info : Analytical Method 3.6.1
Vial Number: 1

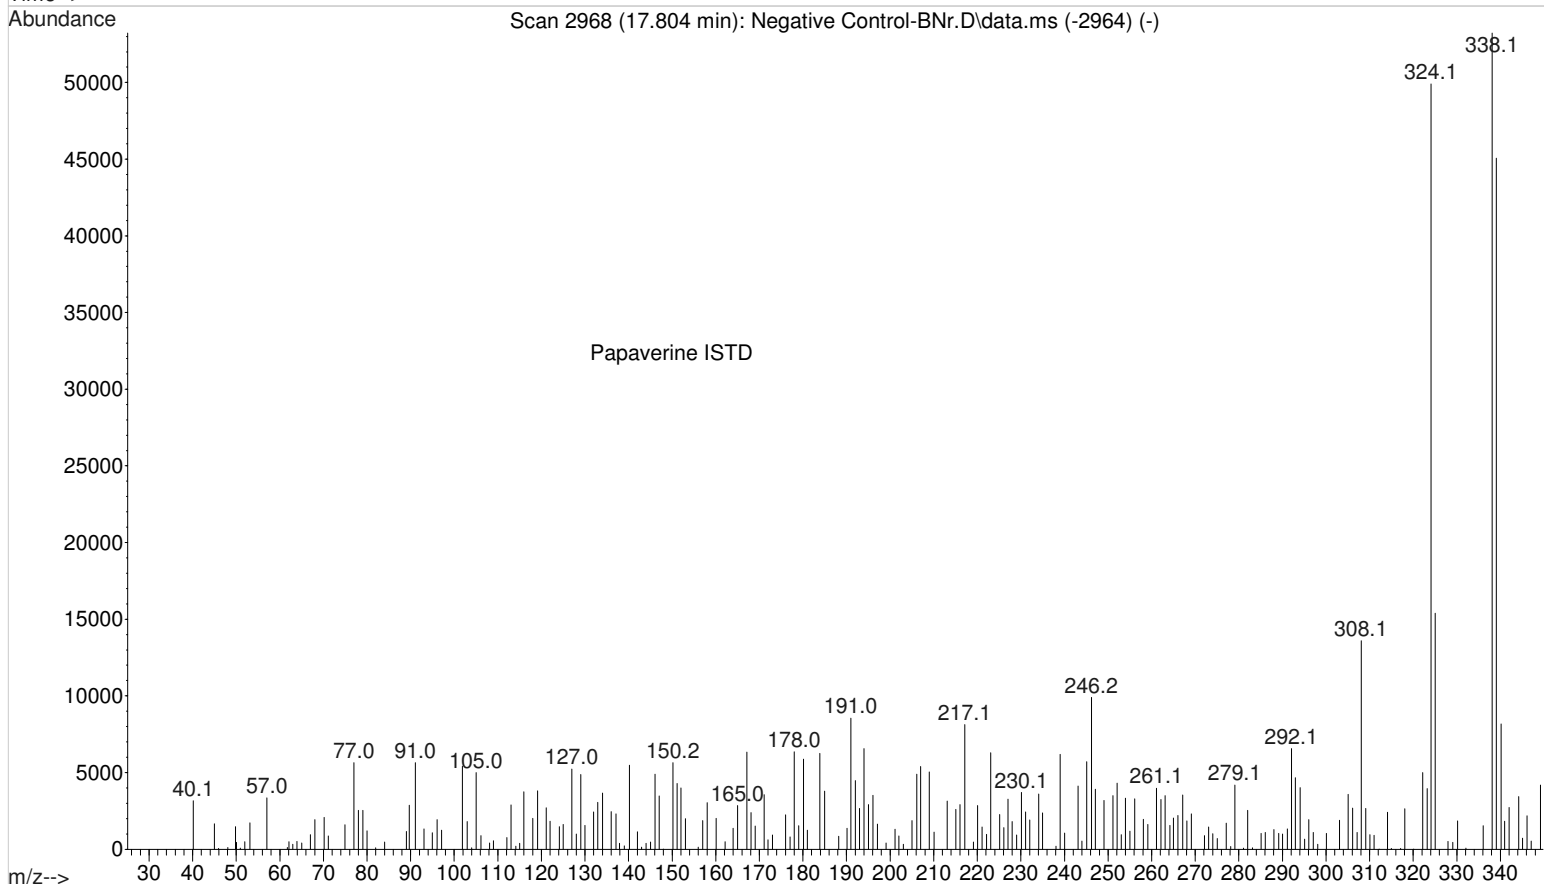
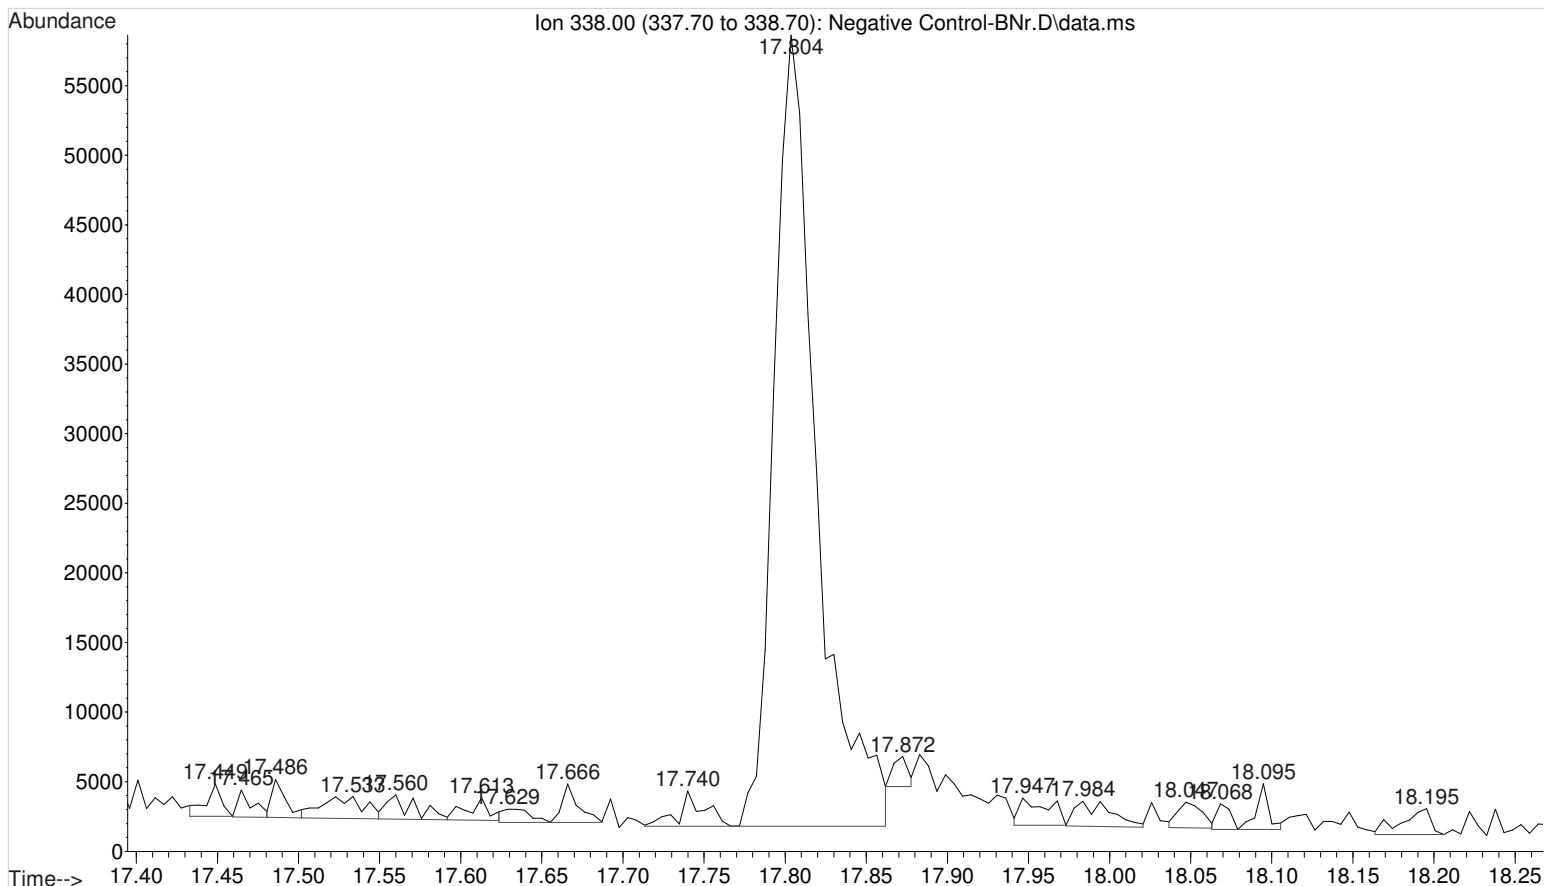


[Handwritten signature]



File :F:\11072016\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 07 Nov 2016 14:28 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

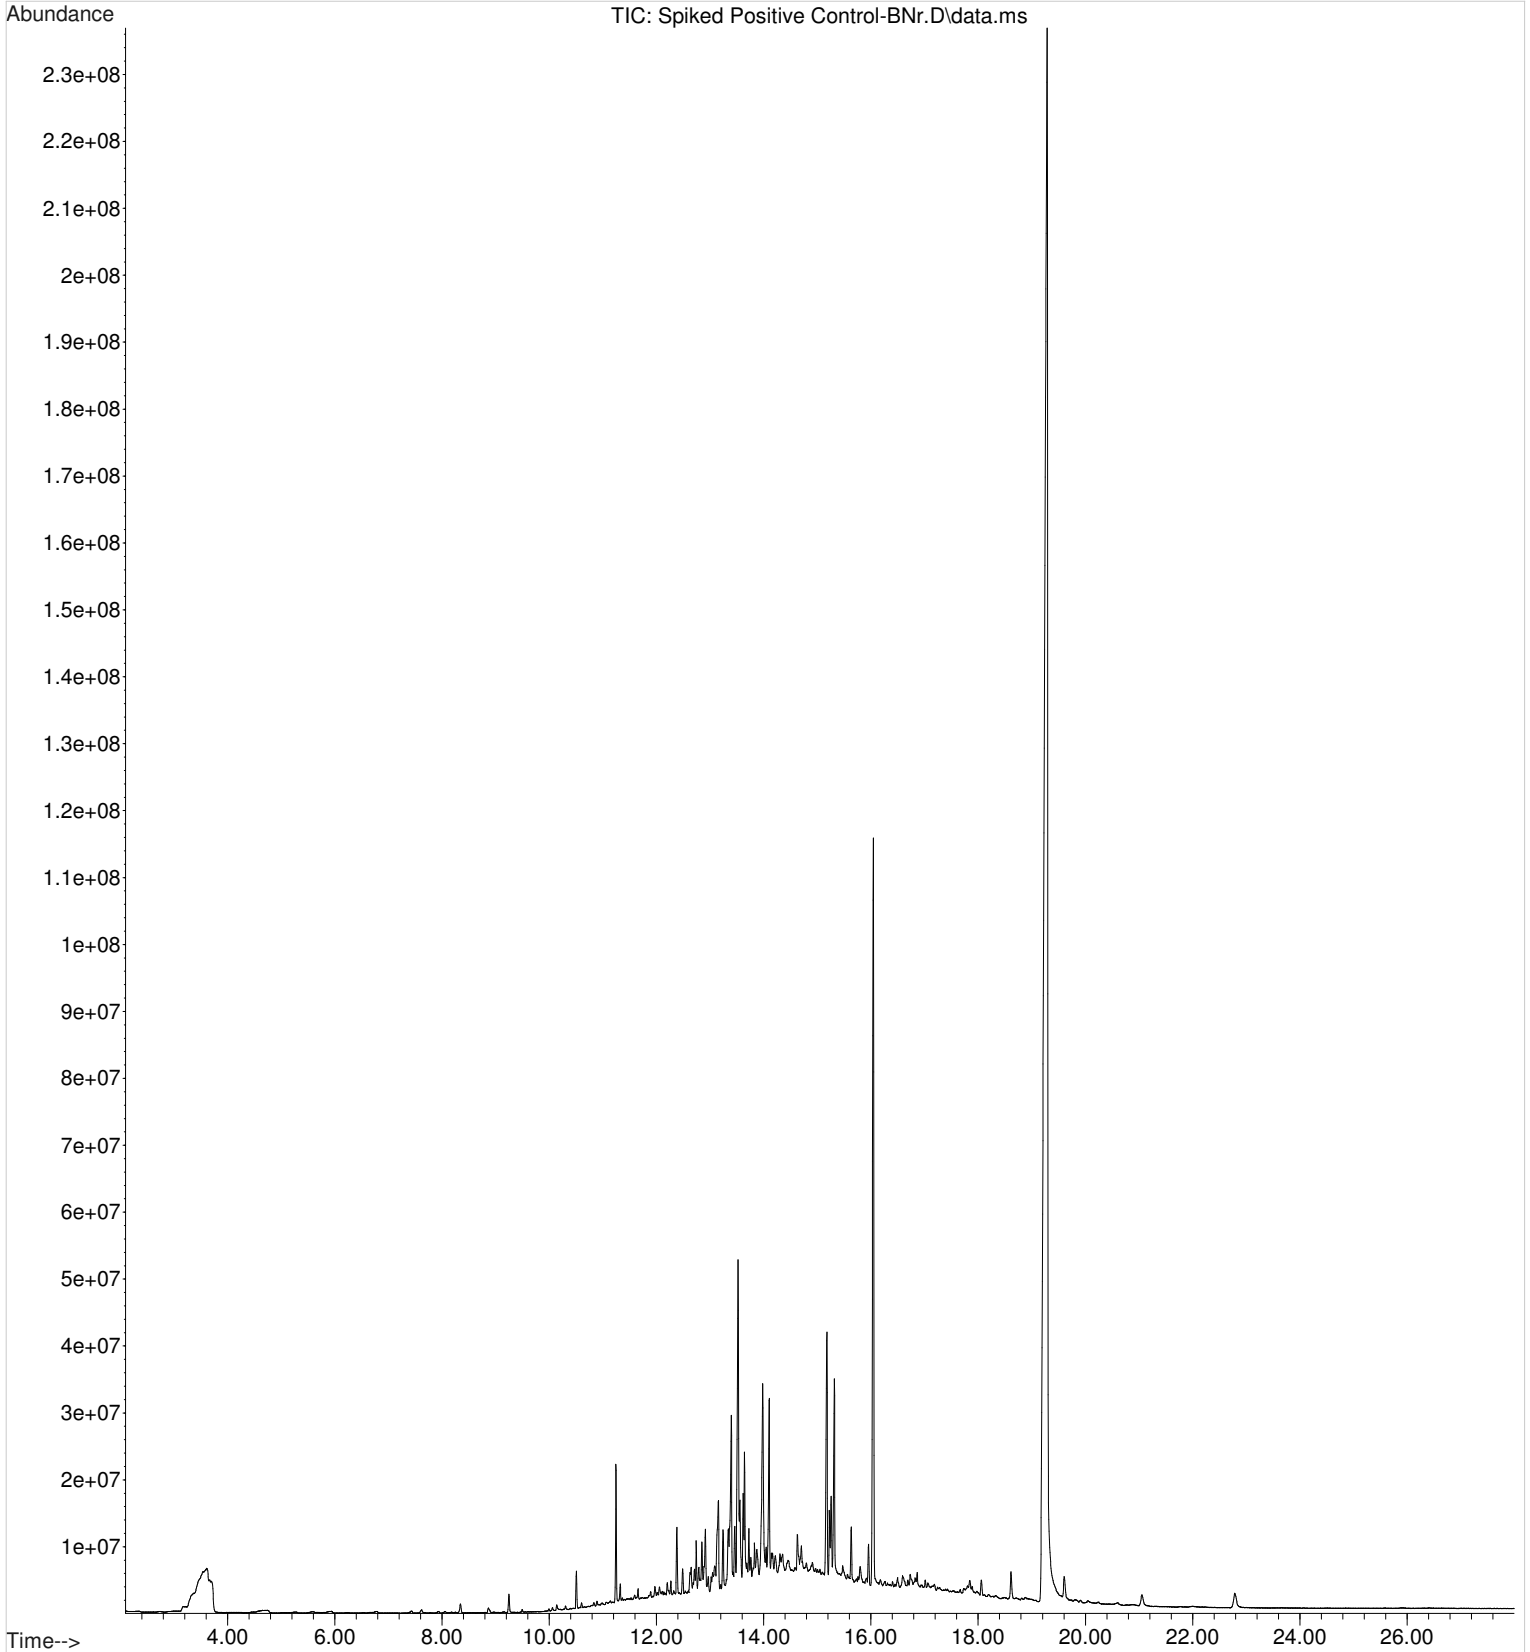



File : F:\11072016\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 07 Nov 2016 14:28 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name : Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

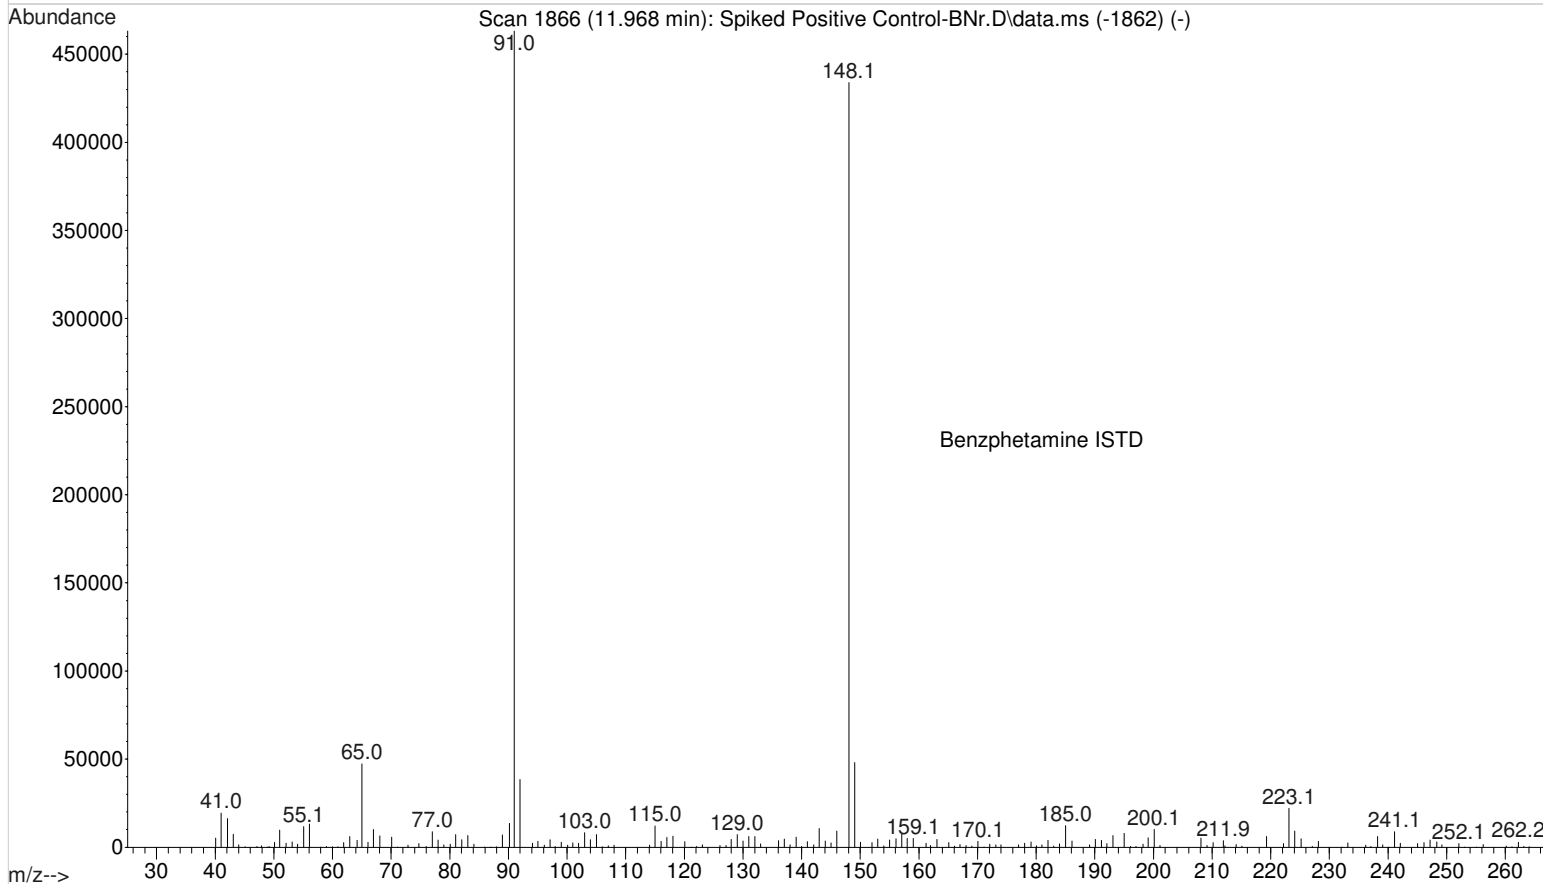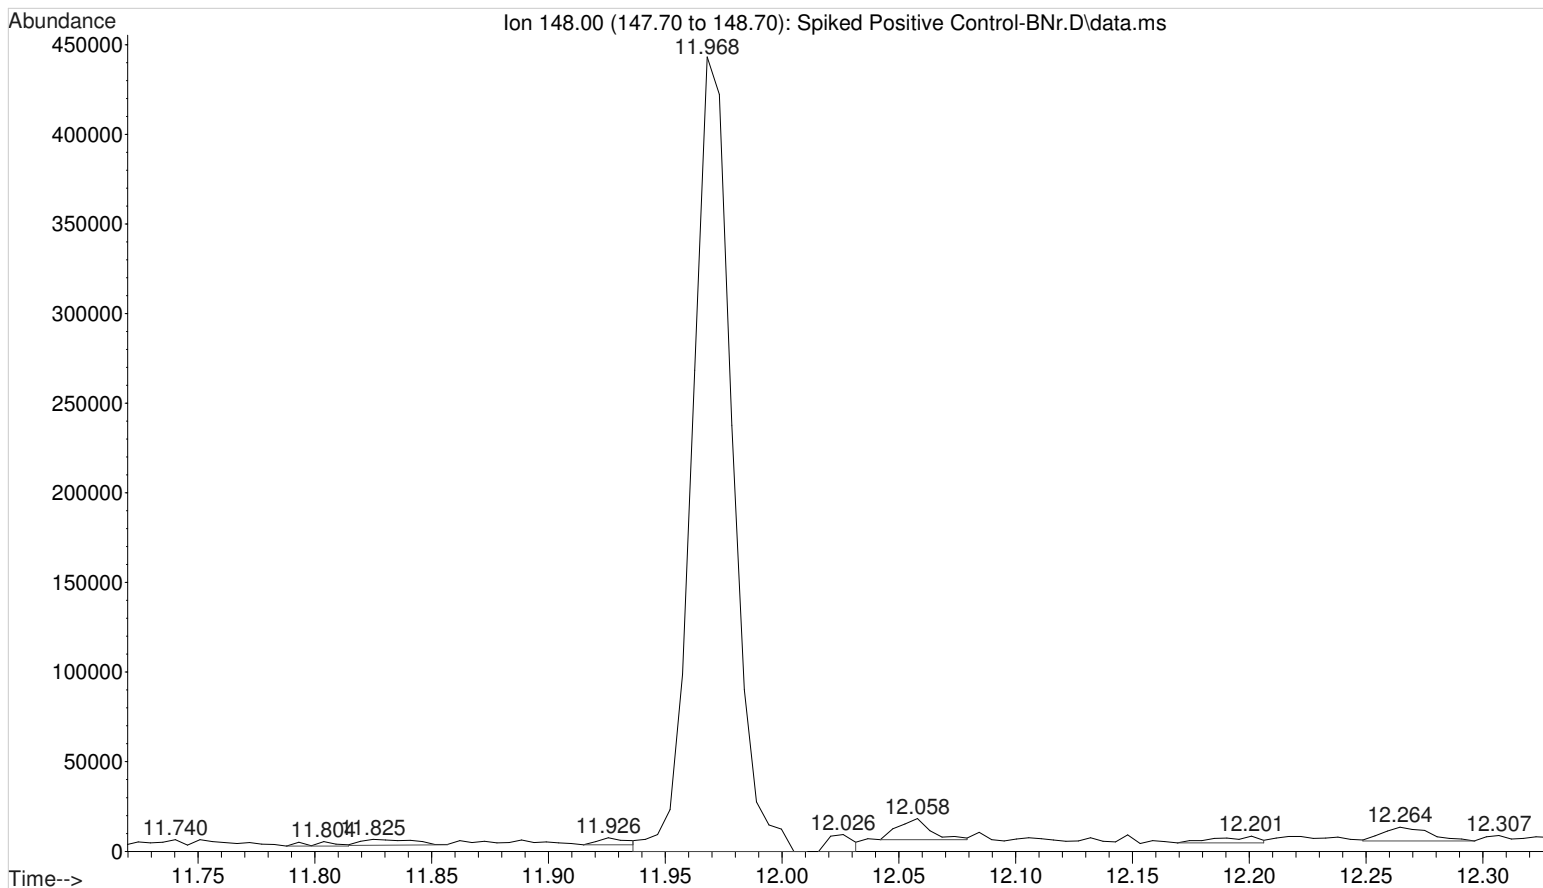



File : F:\11072016\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 07 Nov 2016 14:28 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name : Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

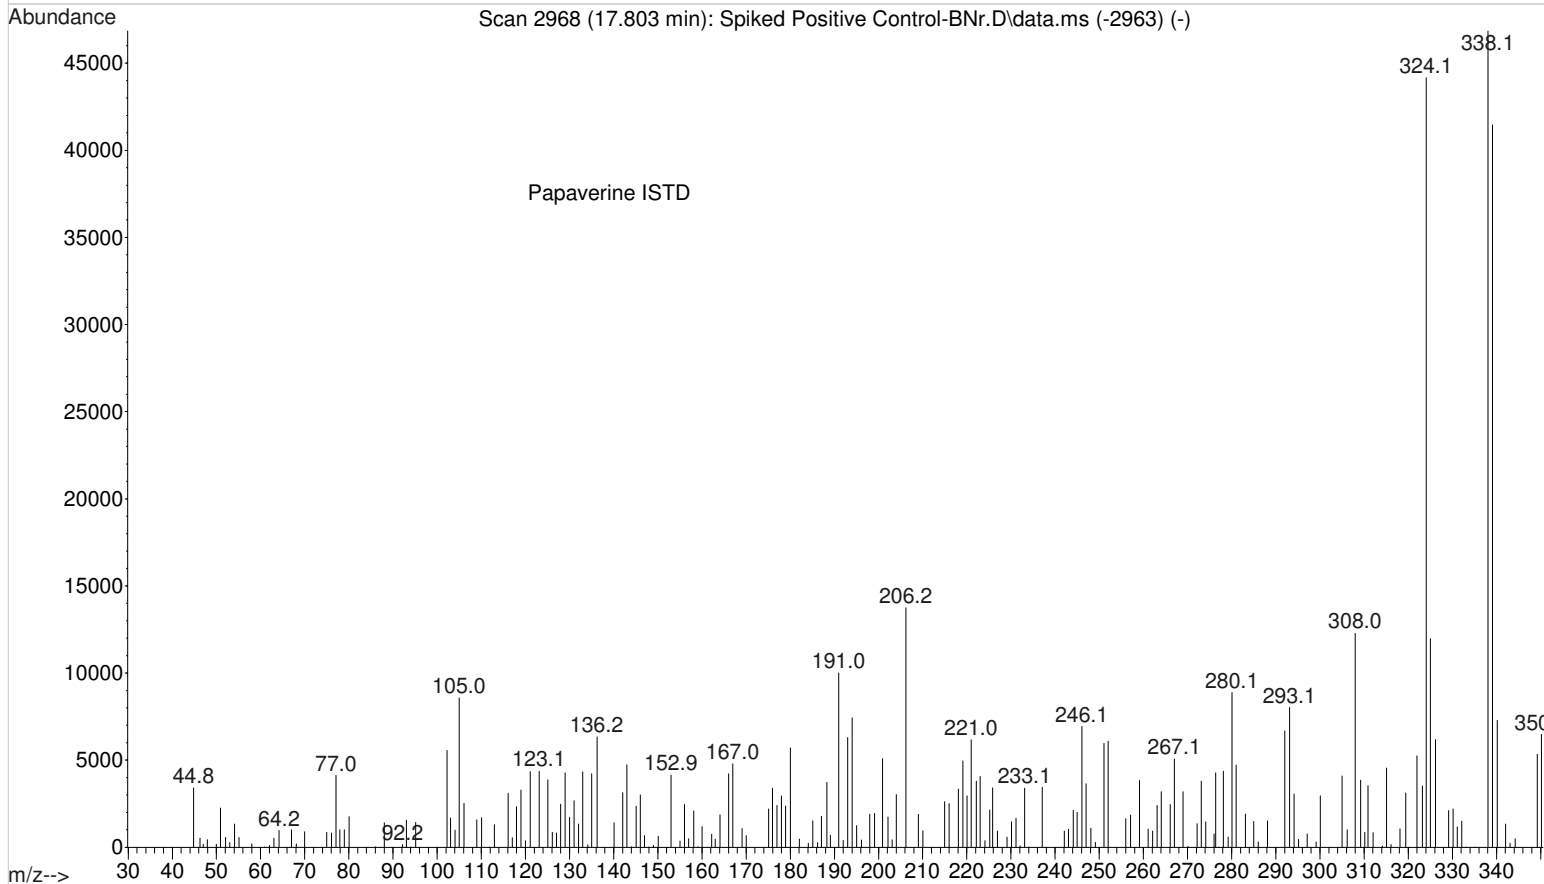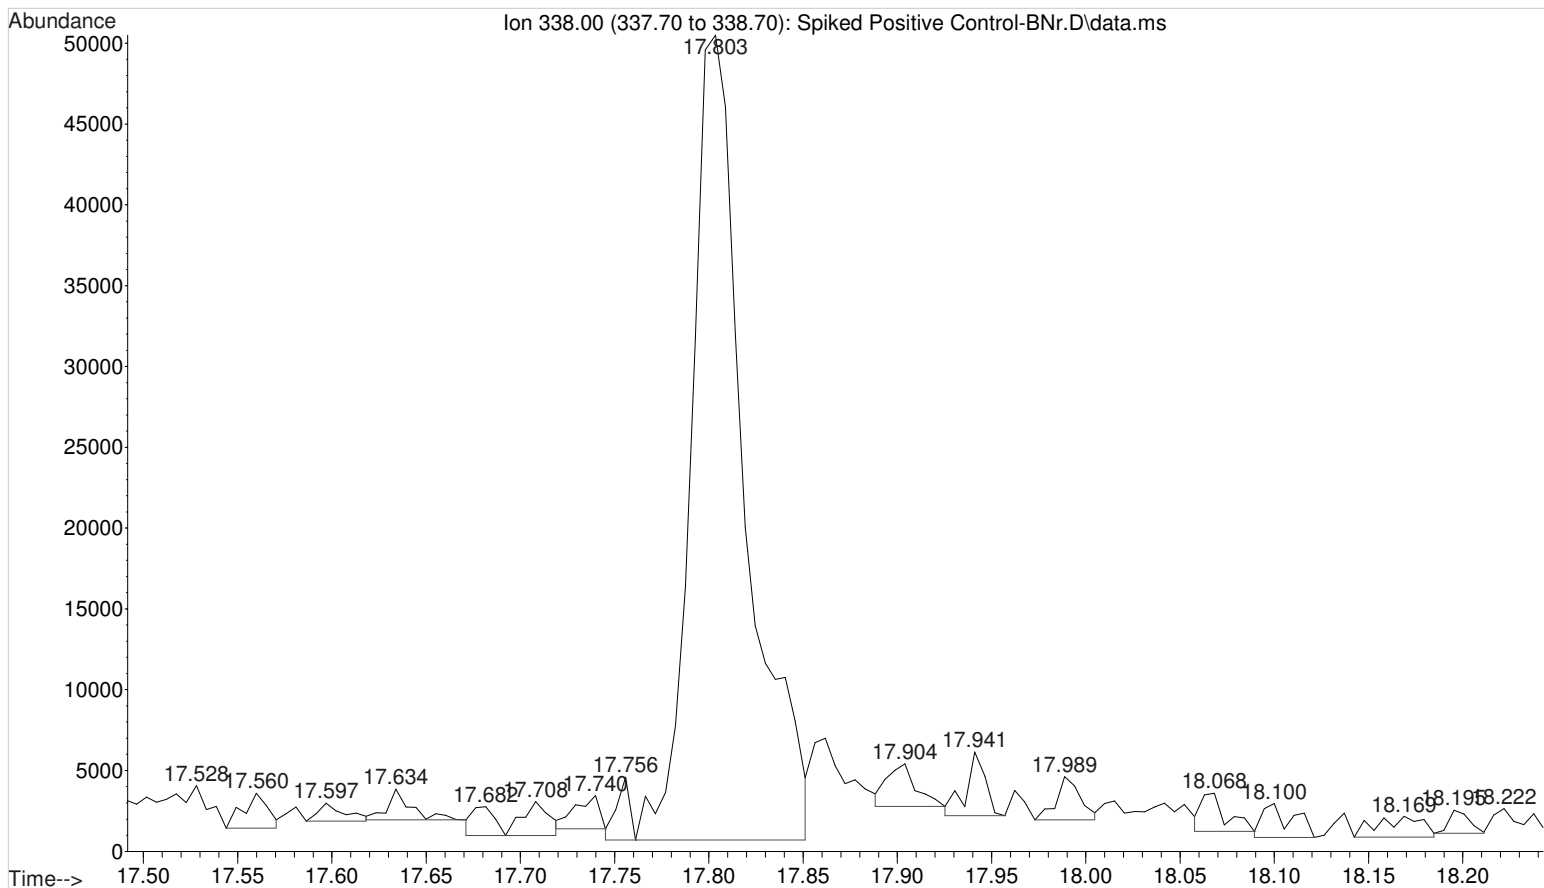



File : F:\11072016\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 07 Nov 2016 14:28 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

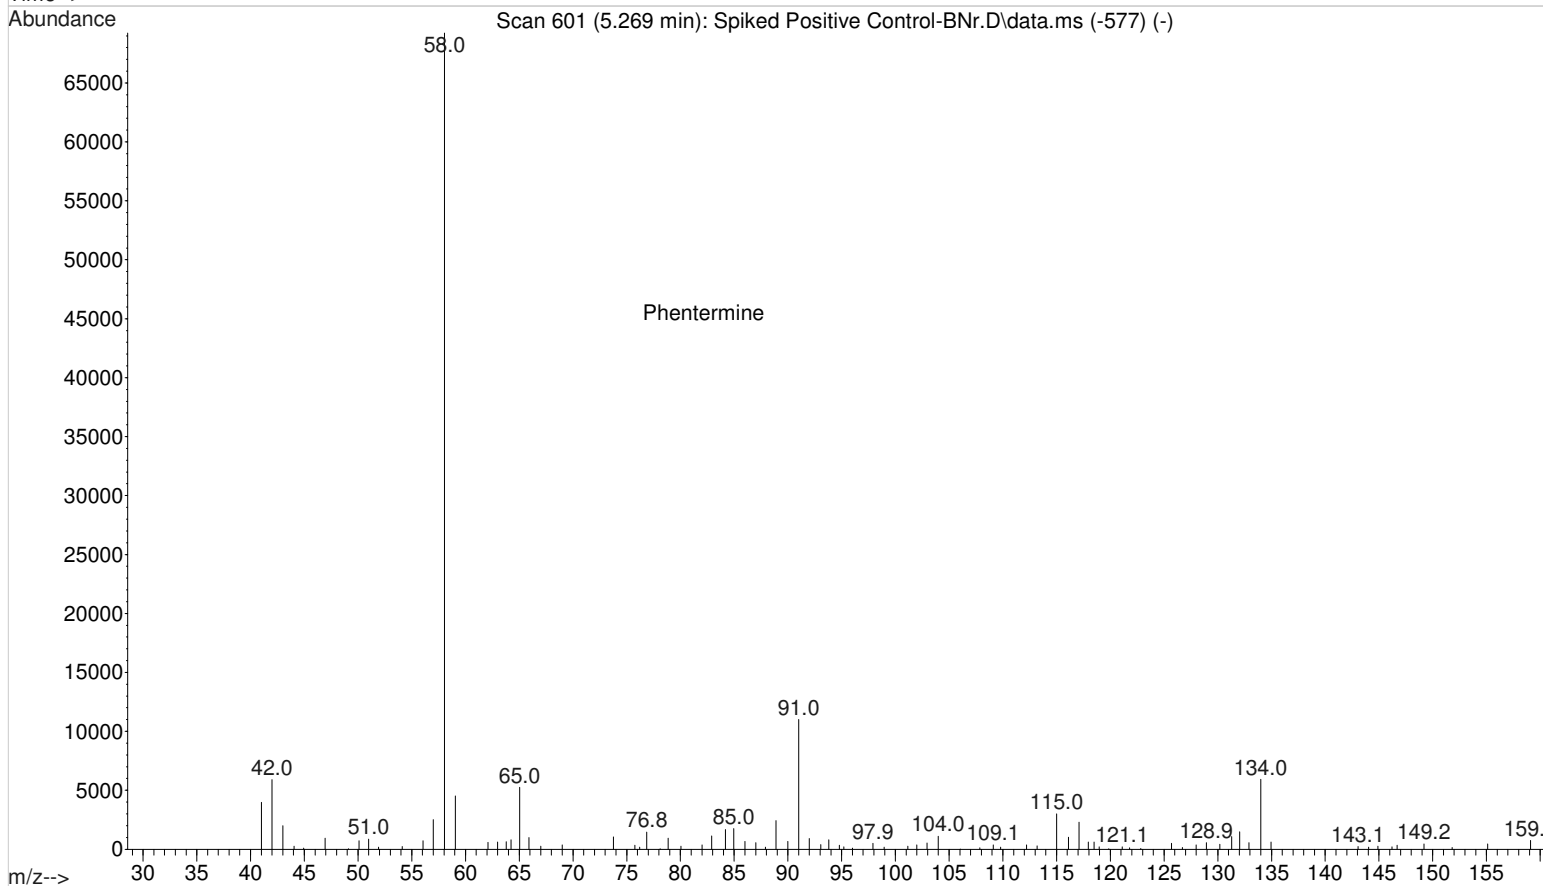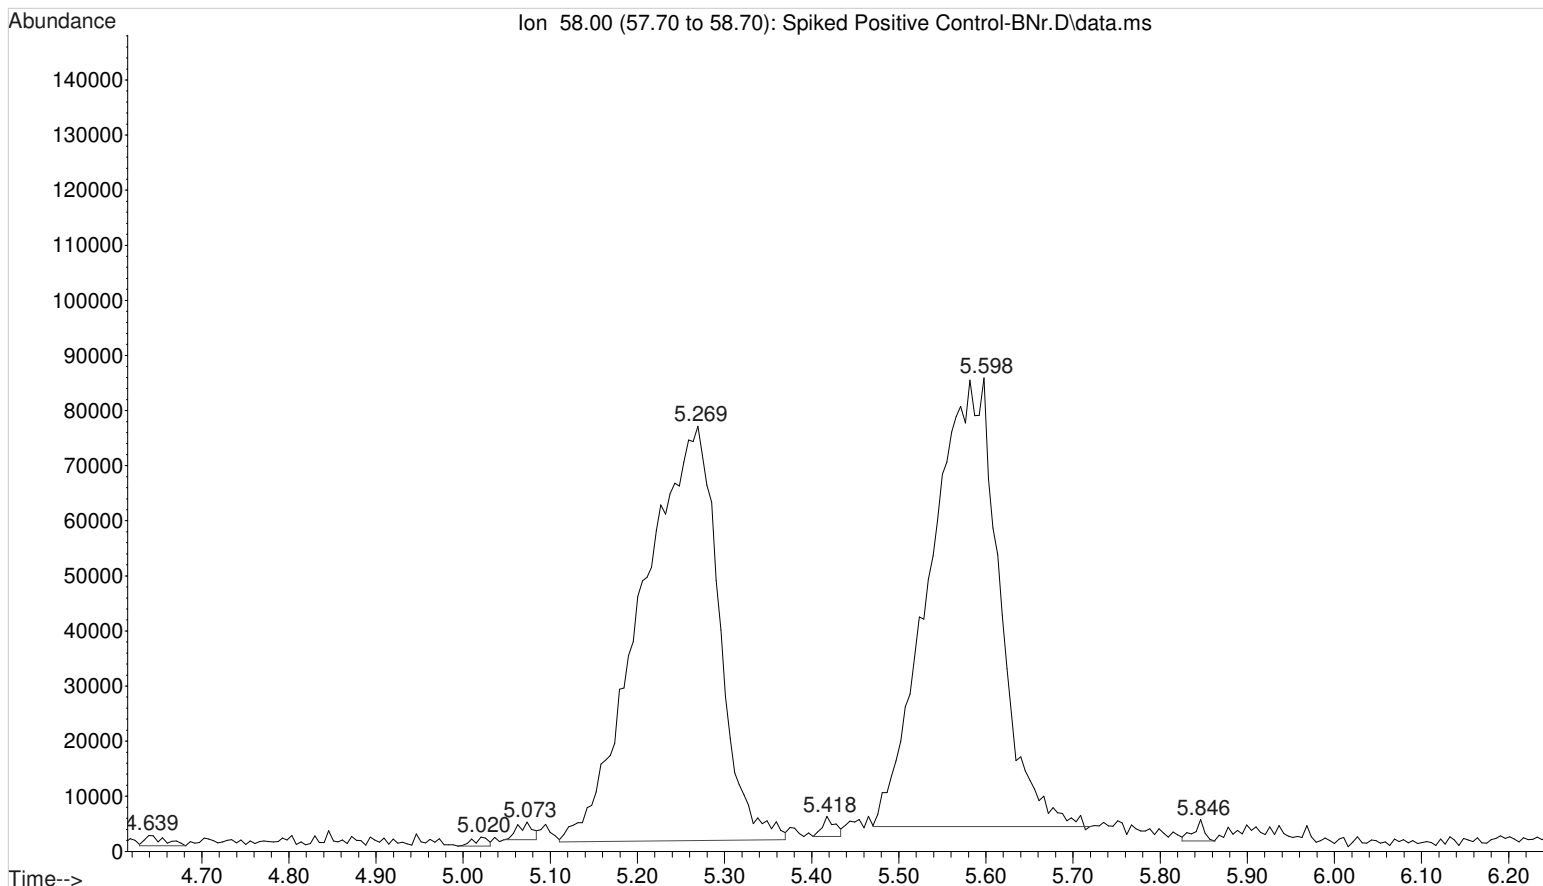



File : F:\11072016\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 07 Nov 2016 14:28 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name : Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

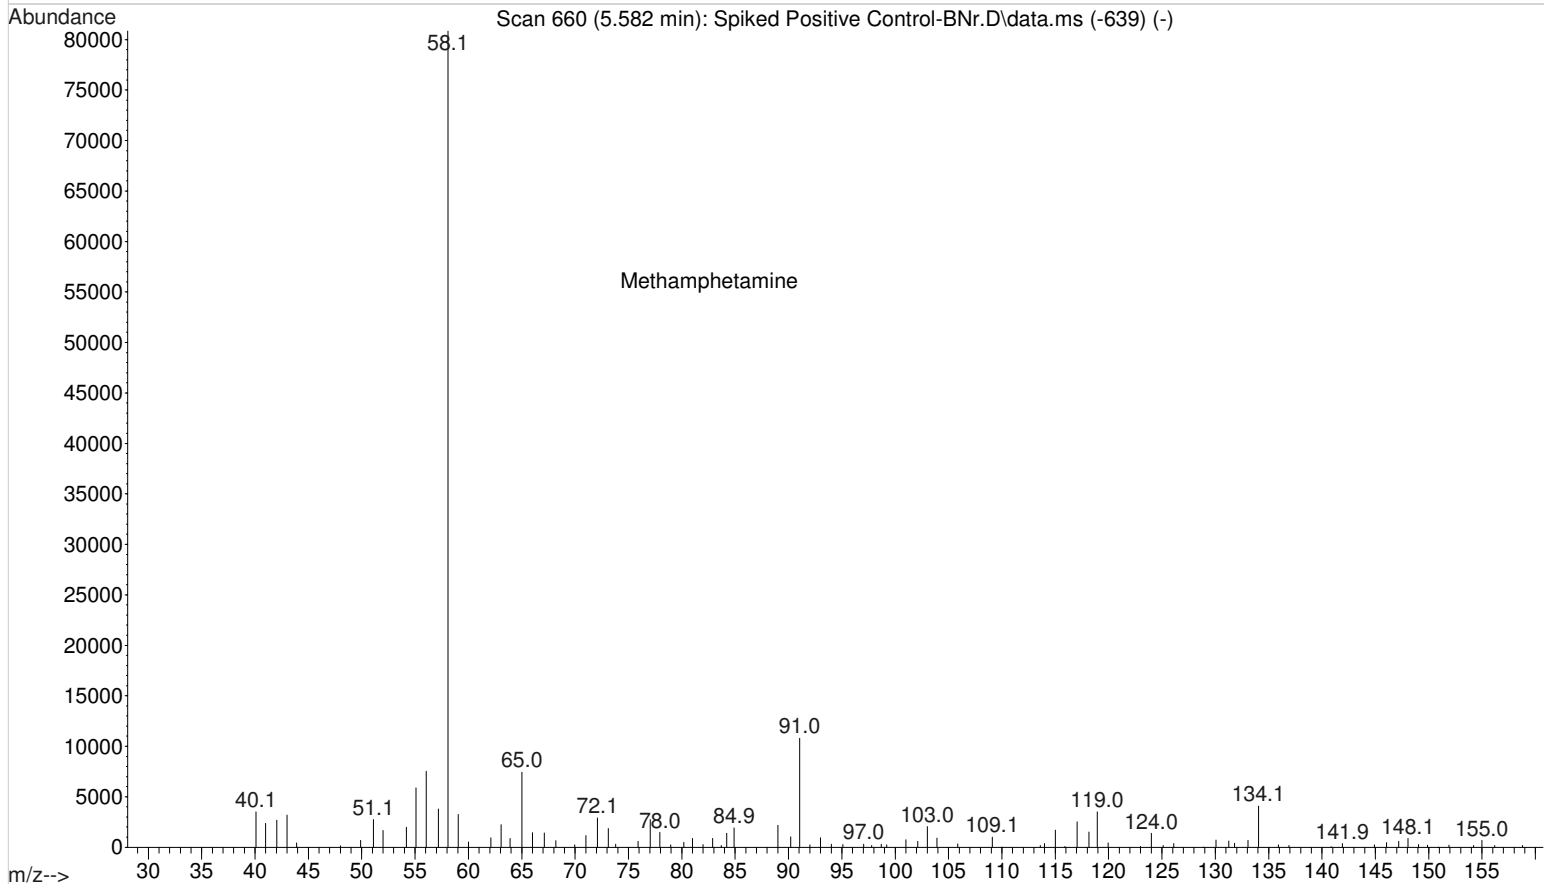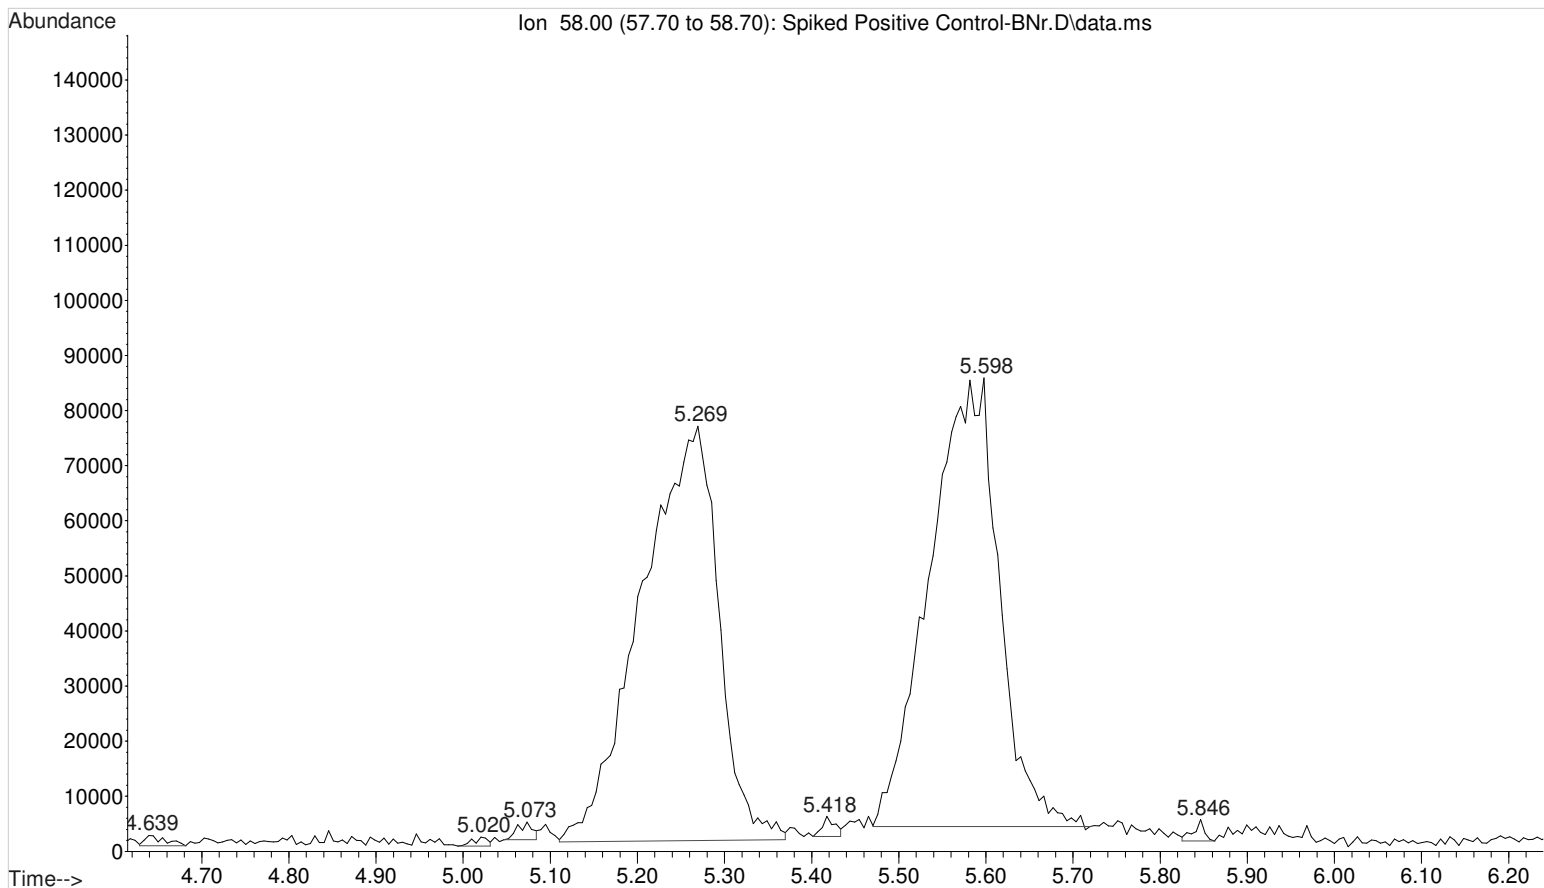

File : F:\11072016\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 07 Nov 2016 14:28 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

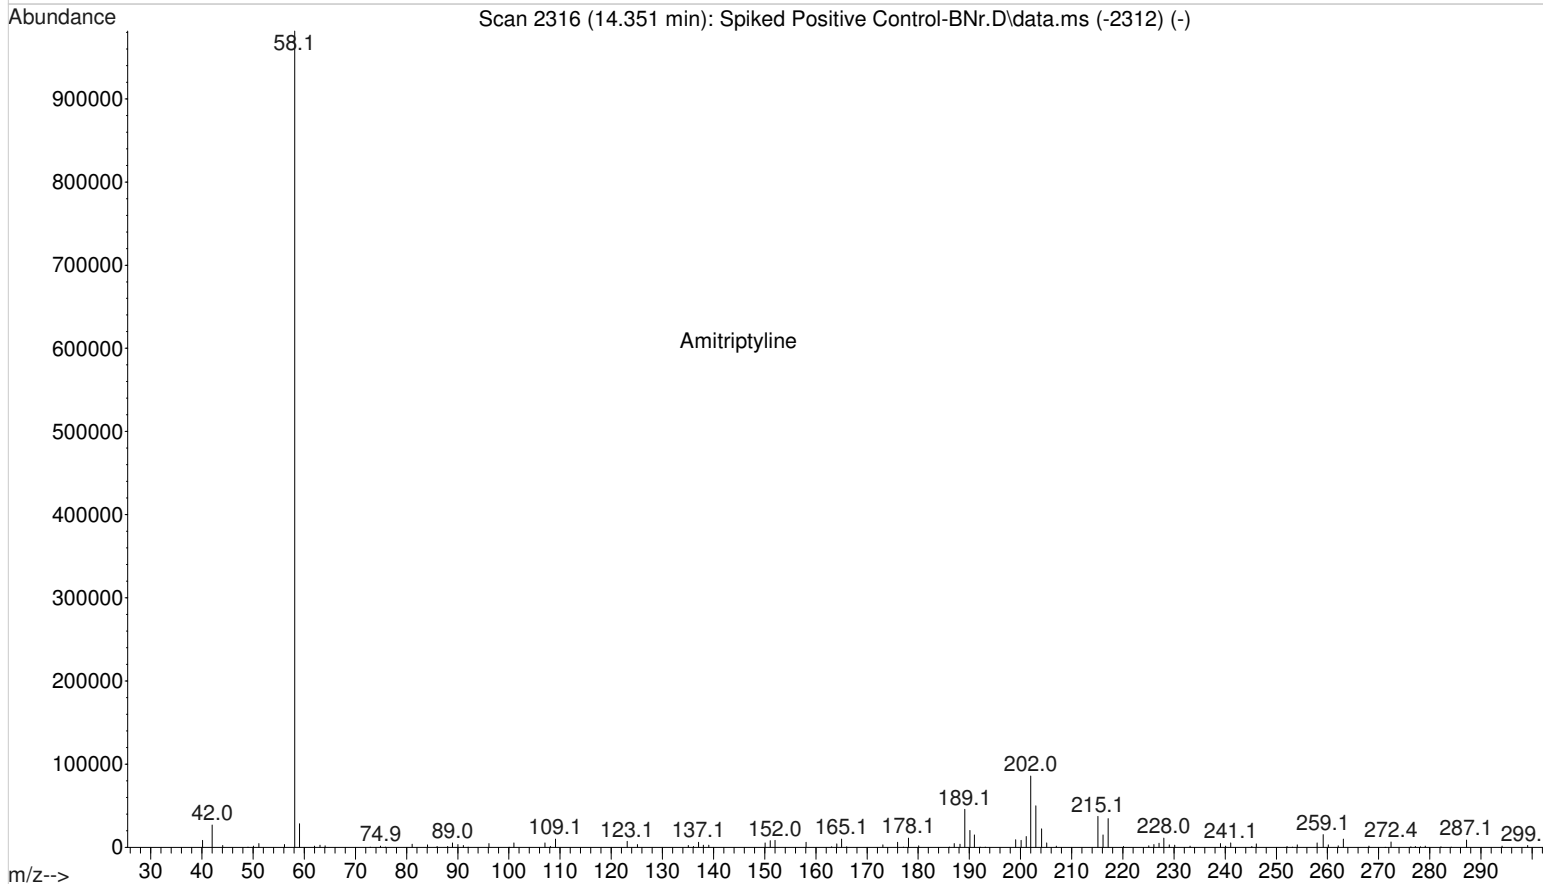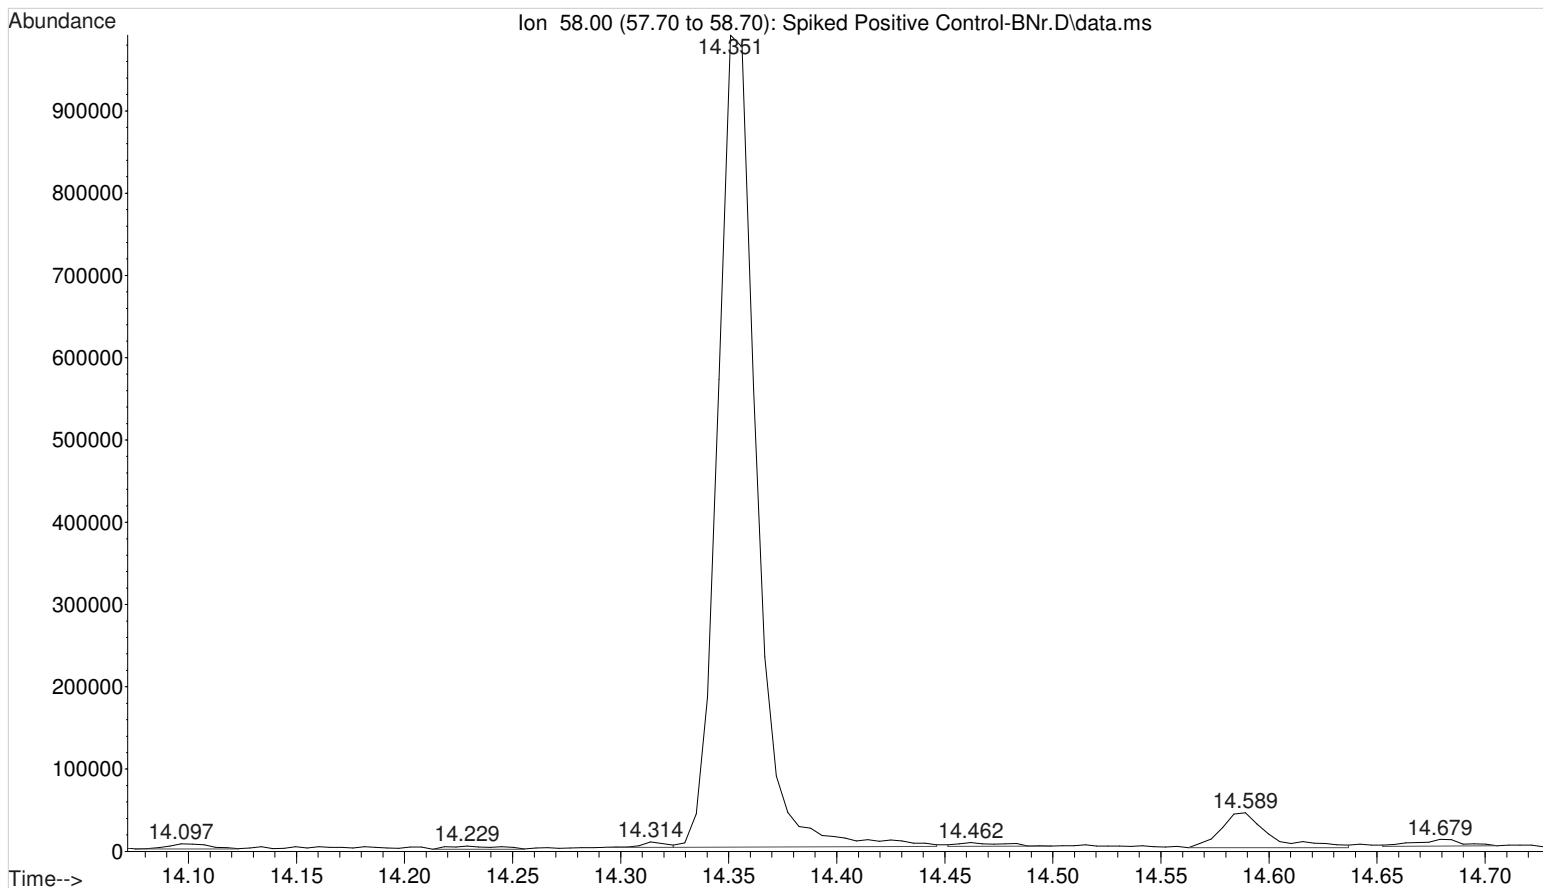

File : F:\11072016\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 07 Nov 2016 14:28 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

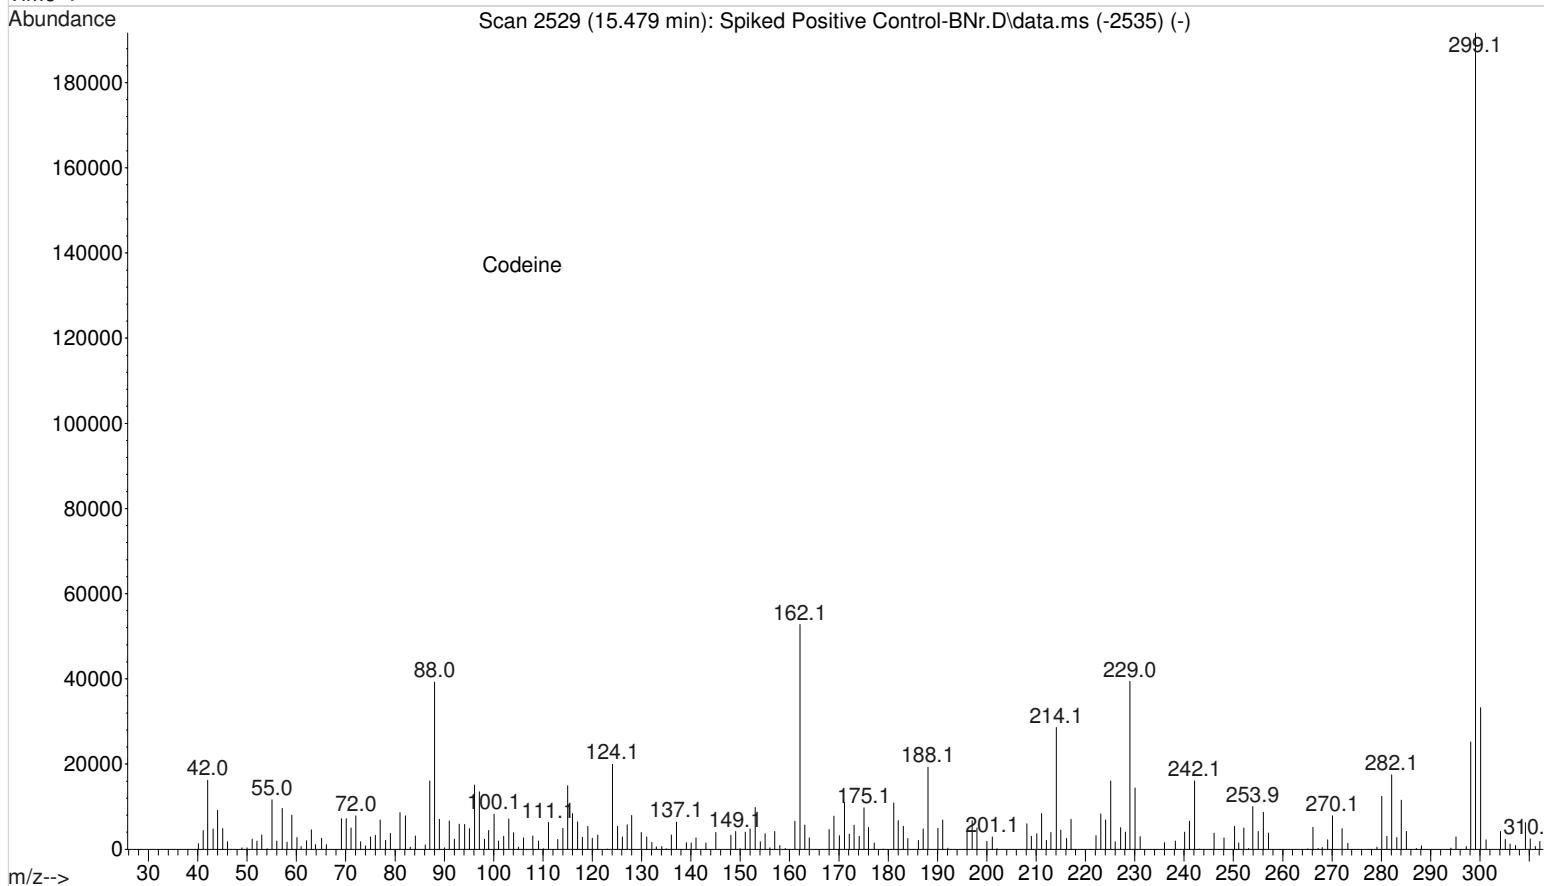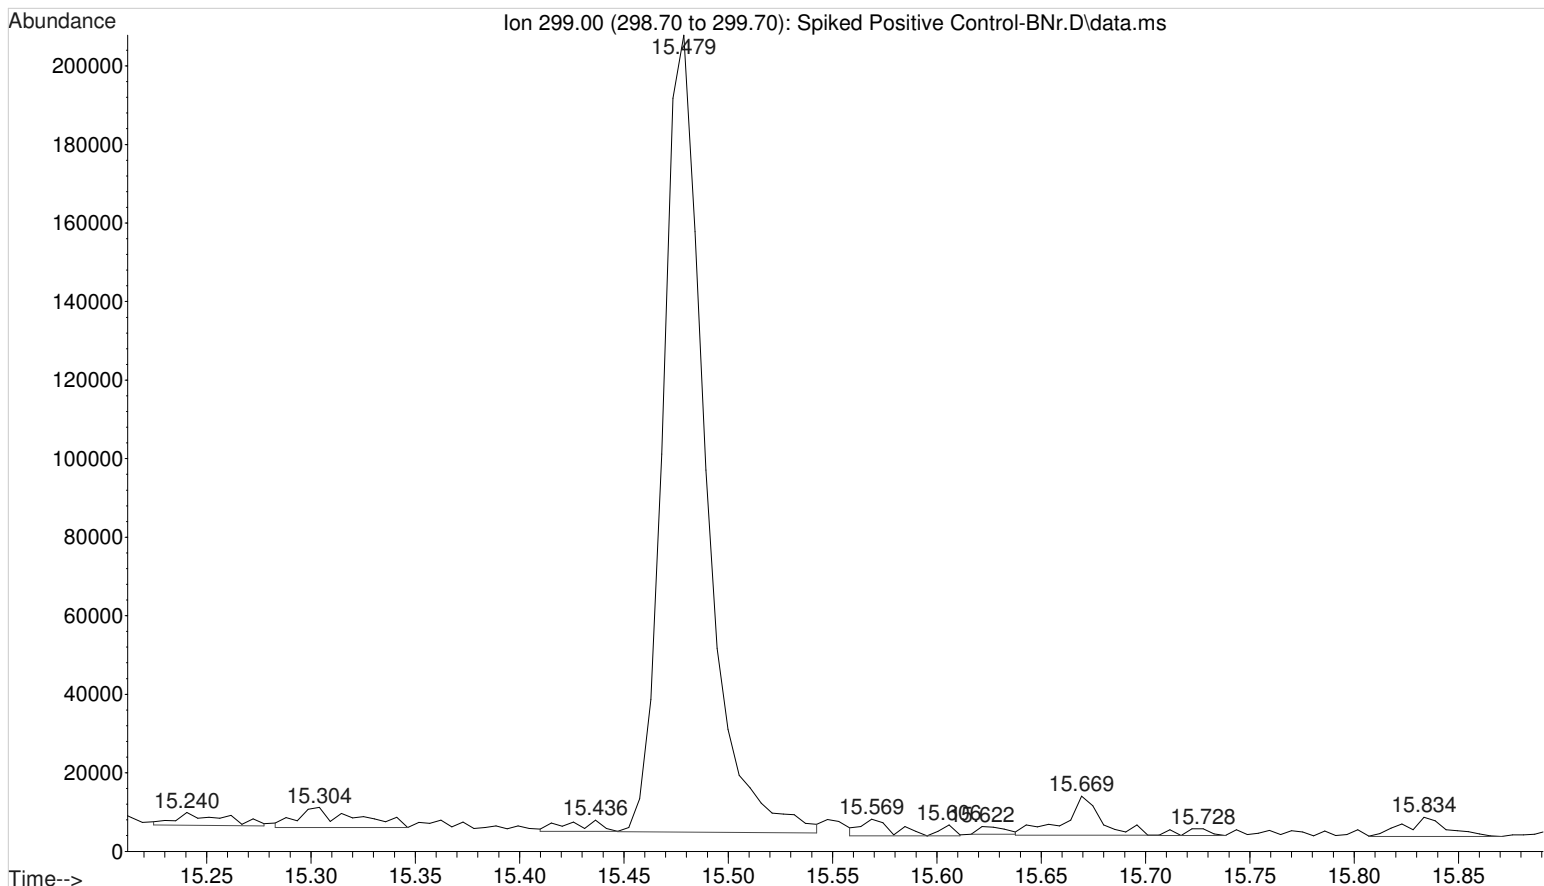

File : F:\11072016\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 07 Nov 2016 14:28 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

