

3/19/2015




Worklist: 630

<u>LAB CASE</u>	<u>ITEM</u>	<u>TASK ID</u>	<u>DESCRIPTION</u>	
M2015-0303	1	27517	3.6.1 Blood base neutral confirr	
M2015-0418	1	28037	3.6.1 Blood base neutral confirr	
M2015-0419	1	28042	3.6.1 Blood base neutral confirr	
M2015-0428	1	28090	3.6.1 Blood base neutral confirr	
M2015-0444	1	28190	3.6.1 Blood base neutral confirr	
M2015-0480	1	28322	3.6.1 Blood base neutral confirr	
P2014-3090	1	29421	3.6.1 Blood base neutral confirr	
P2015-0172	1	29272	3.6.1 Blood base neutral confirr	
P2015-0222	1	26865	3.6.1 Blood base neutral confirr	
P2015-0223	1	26869	3.6.1 Blood base neutral confirr	
P2015-0229	1	29837	3.6.1 Blood base neutral confirr	
P2015-0235	1	26920	3.6.1 Blood base neutral confirr	
P2015-0236	1	26925	3.6.1 Blood base neutral confirr	
P2015-0262	1	27032	3.6.1 Blood base neutral confirr	
P2015-0268	1	27053	3.6.1 Blood base neutral confirr	
P2015-0313	1	27427	3.6.1 Blood base neutral confirr	
P2015-0336	1	27557	3.6.1 Blood base neutral confirr	
P2015-0354	1	27714	3.6.1 Blood base neutral confirr	
P2015-0386	1	27849	3.6.1 Blood base neutral confirr	
P2015-0546	1	28954	3.6.1 Blood base neutral confirr	
P2015-0547	1	28967	3.6.1 Blood base neutral confirr	
P2015-0695	1	30224	3.6.1 Blood base neutral confirr	
P2015-0695	2	30225	3.6.1 Blood base neutral confirr	

POC-AM361

Worklist: 630

<u>LAB_CASE</u>	<u>ITEM</u>	<u>TASK_ID</u>	<u>DESCRIPTION</u>
P2015-0695	3	30226	3.6.1 Blood base neutral confirr



POC_AM 3.6.1_03172015_DND

3/11/15
 DND

simulate_sequence.log
 Simulate Run Sequence Tue Mar 17 15:28:09 2015

Instrument Name: Major Mass Spec
 Sequence File: C:\Users\ISPuser\Desktop\Sequences\DD-BNSB.sequence.xml
 Comment: MassHunter sequence
 Operator: 5LAB-C01\ISPuser
 Data Path: D:\DATA\DND\2015\031715BN\
 Method Path: D:\MassHunter\GCMS\1\methods\

Line	Type	Vials	DataFile	Sample Name
Acquisition Method: BNSB120510.M				
1)	Sample	100 ✓	Prerun Solvent Blank	Pre-run Solvent Blank
2)	Sample	1 ✓	Negative Control-BN	Negative Control -
...	0130			
3)	Sample	2 ✓	Spiked Positive Control-BN	Positive Control
4)	Sample	99 ✓	prbLK2	Solvent Blank
Acquisition Method: GBT092509-Delta EMV.M				
5)	Sample	100 ✓	Prerun Solvent Blankr	Pre-run Solvent Blank
6)	Sample	1 ✓	Negative Control-BNr	Negative Control -
...	0130			
7)	Sample	2 ✓	Spiked Positive Control-BNr	Positive Control
8)	Sample	99 ✓	prbLK2r	Solvent Blank
Acquisition Method: BNSB120510.M				
9)	Sample	98 ✓	P2014-3090-1-BNBLK	Lab No.: P2014-3090-1
10)	Sample	3 ✓	P2014-3090-1-BN	Lab No.: P2014-3090-1
11)	Sample	97 ✓	P2015-0172-1-BNBLK	Lab No.: P2015-0172-1
12)	Sample	4 ✓	P2015-0172-1-BN	Lab No.: P2015-0172-1
13)	Sample	96 ✓	P2015-0222-1-BNBLK	Lab No.: P2015-0222-1
14)	Sample	5 ✓	P2015-0222-1-BN	Lab No.: P2015-0222-1
15)	Sample	95 ✓	P2015-0223-1-BNBLK	Lab No.: P2015-0223-1
16)	Sample	6 ✓	P2015-0223-1-BN	Lab No.: P2015-0223-1
17)	Sample	94 ✓	P2015-0229-1-BNBLK	Lab No.: P2015-0229-1
18)	Sample	7 ✓	P2015-0229-1-BN	Lab No.: P2015-0229-1
19)	Sample	93 ✓	P2015-0235-1-BNBLK	Lab No.: P2015-0235-1
20)	Sample	8 ✓	P2015-0235-1-BN	Lab No.: P2015-0235-1
21)	Sample	92 ✓	P2015-0236-1-BNBLK	Lab No.: P2015-0236-1
22)	Sample	9 ✓	P2015-0236-1-BN	Lab No.: P2015-0236-1
23)	Sample	91 ✓	P2015-0262-1-BNBLK	Lab No.: P2015-0262-1
24)	Sample	10 ✓	P2015-0262-1-BN	Lab No.: P2015-0262-1
Acquisition Method: GBT092509-Delta EMV.M				
25)	Sample	98 ✓	P2014-3090-1-BNBLKr	Lab No.: P2014-3090-1
26)	Sample	3 ✓	P2014-3090-1-BNr	Lab No.: P2014-3090-1
27)	Sample	97 ✓	P2015-0172-1-BNBLKr	Lab No.: P2015-0172-1
28)	Sample	4 ✓	P2015-0172-1-BNr	Lab No.: P2015-0172-1
29)	Sample	96 ✓	P2015-0222-1-BNBLKr	Lab No.: P2015-0222-1
30)	Sample	5 ✓	P2015-0222-1-BNr	Lab No.: P2015-0222-1
31)	Sample	95 ✓	P2015-0223-1-BNBLKr	Lab No.: P2015-0223-1
32)	Sample	6 ✓	P2015-0223-1-BNr	Lab No.: P2015-0223-1
33)	Sample	94 ✓	P2015-0229-1-BNBLKr	Lab No.: P2015-0229-1
34)	Sample	7 ✓	P2015-0229-1-BNr	Lab No.: P2015-0229-1
35)	Sample	93 ✓	P2015-0235-1-BNBLKr	Lab No.: P2015-0235-1
36)	Sample	8 ✓	P2015-0235-1-BNr	Lab No.: P2015-0235-1
37)	Sample	92 ✓	P2015-0236-1-BNBLKr	Lab No.: P2015-0236-1
38)	Sample	9 ✓	P2015-0236-1-BNr	Lab No.: P2015-0236-1
39)	Sample	91 ✓	P2015-0262-1-BNBLKr	Lab No.: P2015-0262-1
40)	Sample	10 ✓	P2015-0262-1-BNr	Lab No.: P2015-0262-1
Acquisition Method: BNSB120510.M				
41)	Sample	90 ✓	P2015-0268-1-BNBLK	Lab No.: P2015-0268-1
42)	Sample	11 ✓	P2015-0268-1-BN	Lab No.: P2015-0268-1
43)	Sample	89 ✓	P2015-0313-1-BNBLK	Lab No.: P2015-0313-1
44)	Sample	12 ✓	P2015-0313-1-BN	Lab No.: P2015-0313-1

03/17/15

simulate_sequence.log
45) Sample 88 ✓ P2015-0336-1-BNBLK Lab No.: P2015-0336-1
46) Sample 13 ✓ P2015-0336-1-BN Lab No.: P2015-0336-1
47) Sample 87 ✓ P2015-0354-1-BNBLK Lab No.: P2015-0354-1
48) Sample 14 ✓ P2015-0354-1-BN Lab No.: P2015-0354-1
49) Sample 86 ✓ P2015-0386-1-BNBLK Lab No.: P2015-0386-1
50) Sample 15 ✓ P2015-0386-1-BN Lab No.: P2015-0386-1

Acquisition Method: GBT092509-Delta EMV.M
51) Sample 90 ✓ P2015-0268-1-BNBLK Lab No.: P2015-0268-1
52) Sample 11 ✓ P2015-0268-1-BNr Lab No.: P2015-0268-1
53) Sample 89 ✓ P2015-0313-1-BNBLK Lab No.: P2015-0313-1
54) Sample 12 ✓ P2015-0313-1-BNr Lab No.: P2015-0313-1
55) Sample 88 ✓ P2015-0336-1-BNBLK Lab No.: P2015-0336-1
56) Sample 13 ✓ P2015-0336-1-BNr Lab No.: P2015-0336-1
57) Sample 87 ✓ P2015-0354-1-BNBLK Lab No.: P2015-0354-1
58) Sample 14 ✓ P2015-0354-1-BNr Lab No.: P2015-0354-1
59) Sample 86 ✓ P2015-0386-1-BNBLK Lab No.: P2015-0386-1
60) Sample 15 ✓ P2015-0386-1-BNr Lab No.: P2015-0386-1

Acquisition Method: BNSB120510.M
61) Sample 85 ✓ P2015-0546-1-BNBLK Lab No.: P2015-0546-1
62) Sample 16 ✓ P2015-0546-1-BN Lab No.: P2015-0546-1
63) Sample 84 ✓ P2015-0547-1-BNBLK Lab No.: P2015-0547-1
64) Sample 17 ✓ P2015-0547-1-BN Lab No.: P2015-0547-1
65) Sample 83 ✓ P2015-0695-1-BNBLK Lab No.: P2015-0695-1
66) Sample 18 ✓ P2015-0695-1-BN Lab No.: P2015-0695-1
67) Sample 82 ✓ P2015-0695-2-BNBLK Lab No.: P2015-0695-2
68) Sample 19 ✓ P2015-0695-2-BN Lab No.: P2015-0695-2
69) Sample 81 ✓ P2015-0695-3-BNBLK Lab No.: P2015-0695-3
70) Sample 20 ✓ P2015-0695-3-BN Lab No.: P2015-0695-3

Acquisition Method: GBT092509-Delta EMV.M
71) Sample 85 ✓ P2015-0546-1-BNBLK Lab No.: P2015-0546-1
72) Sample 16 ✓ P2015-0546-1-BNr Lab No.: P2015-0546-1
73) Sample 84 ✓ P2015-0547-1-BNBLK Lab No.: P2015-0547-1
74) Sample 17 ✓ P2015-0547-1-BNr Lab No.: P2015-0547-1
75) Sample 83 ✓ P2015-0695-1-BNBLK Lab No.: P2015-0695-1
76) Sample 18 ✓ P2015-0695-1-BNr Lab No.: P2015-0695-1
77) Sample 82 ✓ P2015-0695-2-BNBLK Lab No.: P2015-0695-2
78) Sample 19 ✓ P2015-0695-2-BNr Lab No.: P2015-0695-2
79) Sample 81 ✓ P2015-0695-3-BNBLK Lab No.: P2015-0695-3
80) Sample 20 ✓ P2015-0695-3-BNr Lab No.: P2015-0695-3

Acquisition Method: BNSB120510.M
81) Sample 80 ✓ M2015-0303-1-BNBLK Lab No.: M2015-0303-1
82) Sample 21 ✓ M2015-0303-1-BN Lab No.: M2015-0303-1
83) Sample 79 ✓ M2015-0418-1-BNBLK Lab No.: M2015-0418-1
84) Sample 22 ✓ M2015-0418-1-BN Lab No.: M2015-0418-1
85) Sample 78 ✓ M2015-0419-1-BNBLK Lab No.: M2015-0419-1
86) Sample 23 ✓ M2015-0419-1-BN Lab No.: M2015-0419-1
87) Sample 77 ✓ M2015-0428-1-BNBLK Lab No.: M2015-0428-1
88) Sample 24 ✓ M2015-0428-1-BN Lab No.: M2015-0428-1
89) Sample 76 ✓ M2015-0444-1-BNBLK Lab No.: M2015-0444-1
90) Sample 25 ✓ M2015-0444-1-BN Lab No.: M2015-0444-1

Acquisition Method: GBT092509-Delta EMV.M
91) Sample 80 ✓ M2015-0303-1-BNBLK Lab No.: M2015-0303-1
92) Sample 21 ✓ M2015-0303-1-BNr Lab No.: M2015-0303-1
93) Sample 79 ✓ M2015-0418-1-BNBLK Lab No.: M2015-0418-1
94) Sample 22 ✓ M2015-0418-1-BNr Lab No.: M2015-0418-1
95) Sample 78 ✓ M2015-0419-1-BNBLK Lab No.: M2015-0419-1
96) Sample 23 ✓ M2015-0419-1-BNr Lab No.: M2015-0419-1
97) Sample 77 ✓ M2015-0428-1-BNBLK Lab No.: M2015-0428-1
98) Sample 24 ✓ M2015-0428-1-BNr Lab No.: M2015-0428-1
99) Sample 76 ✓ M2015-0444-1-BNBLK Lab No.: M2015-0444-1
100) Sample 25 ✓ M2015-0444-1-BNr Lab No.: M2015-0444-1

Acquisition Method: BNSB120510.M

or 03/17/15

simulate_sequence.log
101) Sample 75 ✓ M2015-0480-1-BNBLK Lab No.: M2015-0480-1
102) Sample 26 ✓ M2015-0480-1-BN Lab No.: M2015-0480-1

Acquisition Method: GBT092509-Delta EMV.M
103) Sample 75 ✓ M2015-0480-1-BNBLK Lab No.: M2015-0480-1
104) Sample 26 ✓ M2015-0480-1-BNr Lab No.: M2015-0480-1

Acquisition Method: BNSB120510.M
105) Sample 74 ✓ POSTBLK BLK

Acquisition Method: GBT092509-Delta EMV.M
106) Sample 73 ✓ AFTER BLK
megabytes Needed: 2092 Space on drive D: 310122
Sequence Verification Done!

POC_AM 3.6.1_03172015-DND

Analytical Method 3.6.1 & 3.6.7 QA Check List

Run Start Date: 03/17/15

Analyst: DND

(Short GC/MS temperature program)

Positive Control Compound List

- Methamphetamine
- Nicotine
- Meperidine
- Caffeine
- Diphenhydramine
- Lidocaine
- PCP
- Methadone
- Amitriptyline
- Codeine
- Trazodone



Internal Standards

- Benzphetamine
- Papaverine


Optional back extraction **not** performed.
Samples reconstituted in methanol.

POC_AM_3.6.1_03172015_DND



File :C:\gcms\1\data\Blood\031715BN\Prerun Solvent Blank.D
Operator : 5LAB-C01\ISPuser
Acquired : 17 Mar 2015 17:38 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Pre-run Solvent Blank
Misc Info : Chloroform
Vial Number: 100

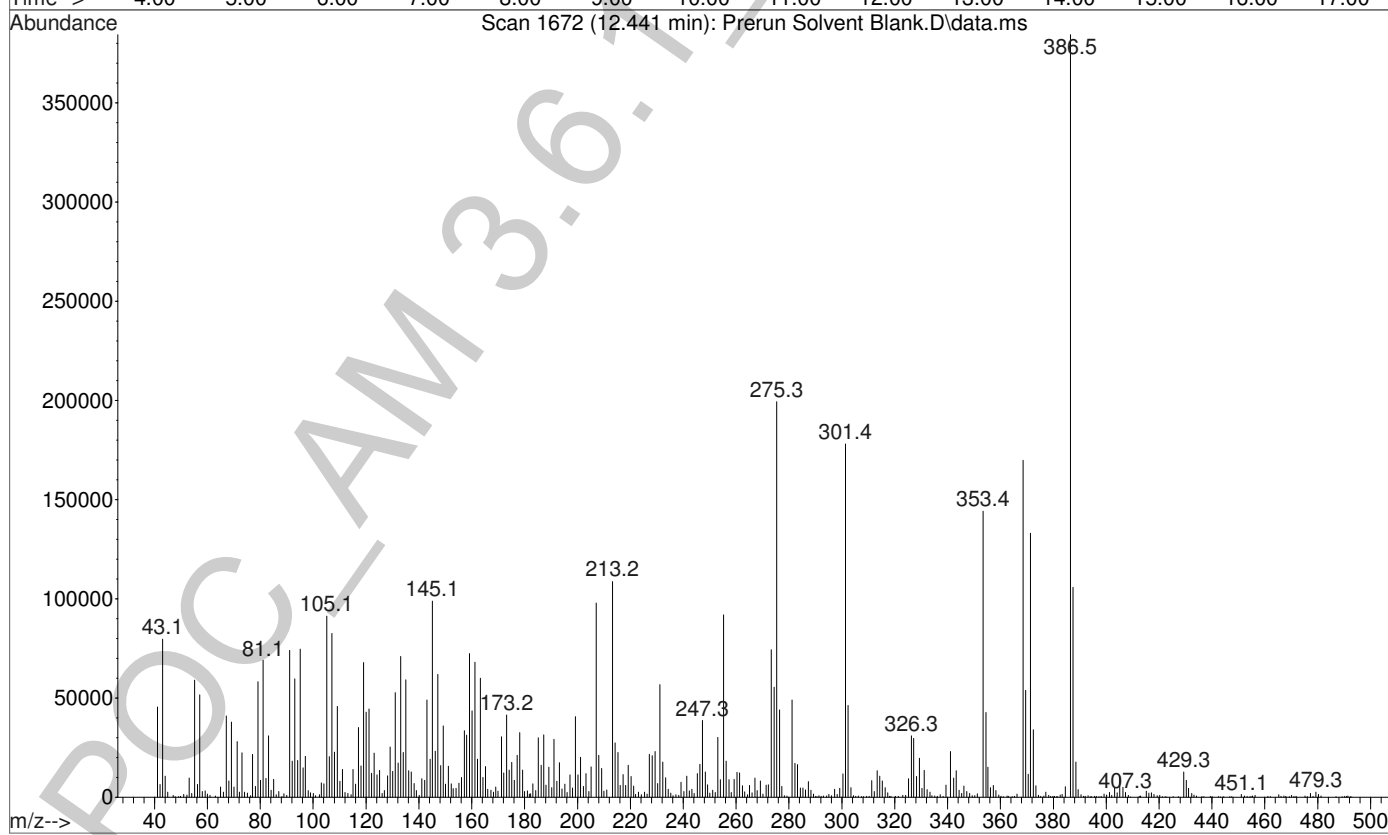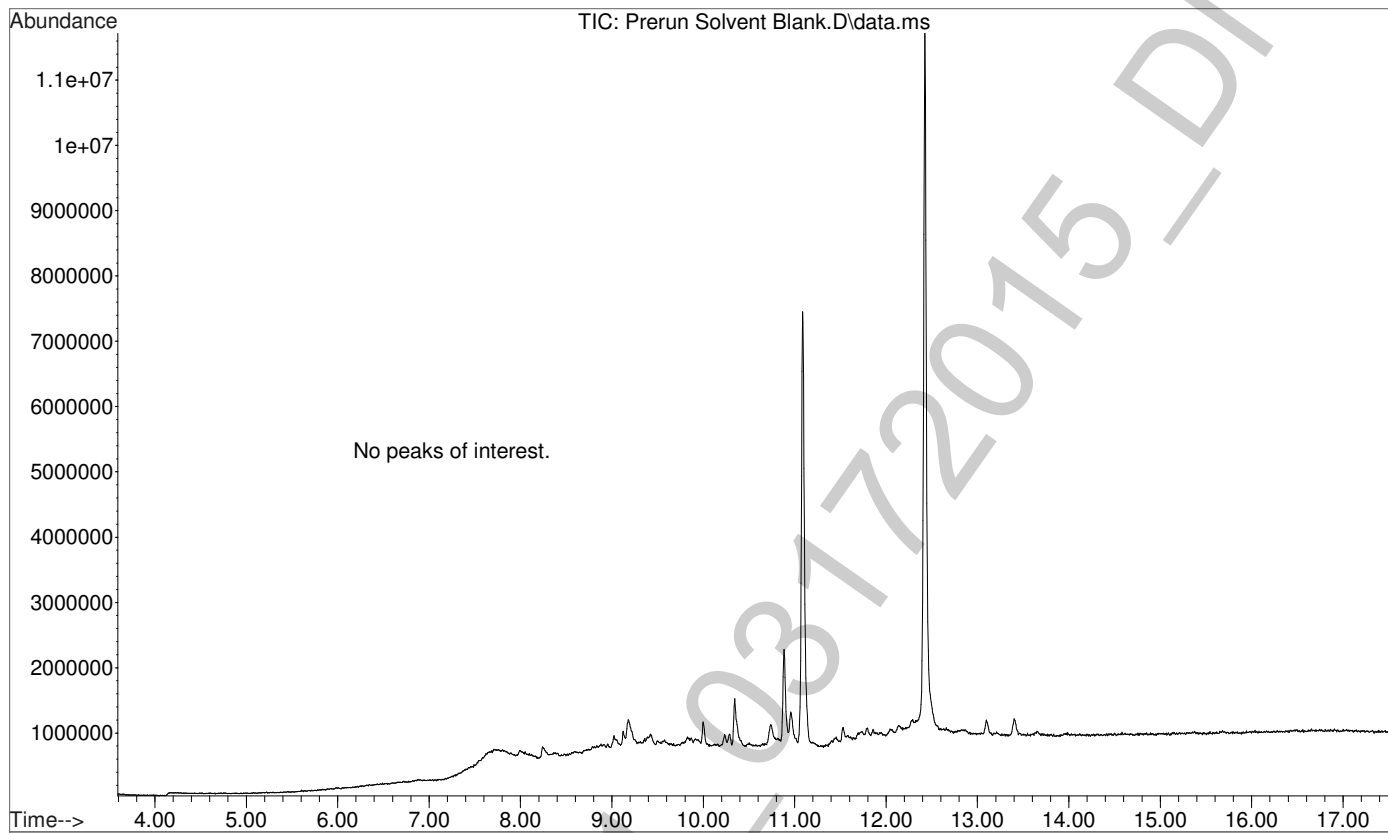



File :C:\gcms\1\data\Blood\031715BN\Negative Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 17 Mar 2015 18:01 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0130
Misc Info : Analytical Method 3.6.1
Vial Number: 1

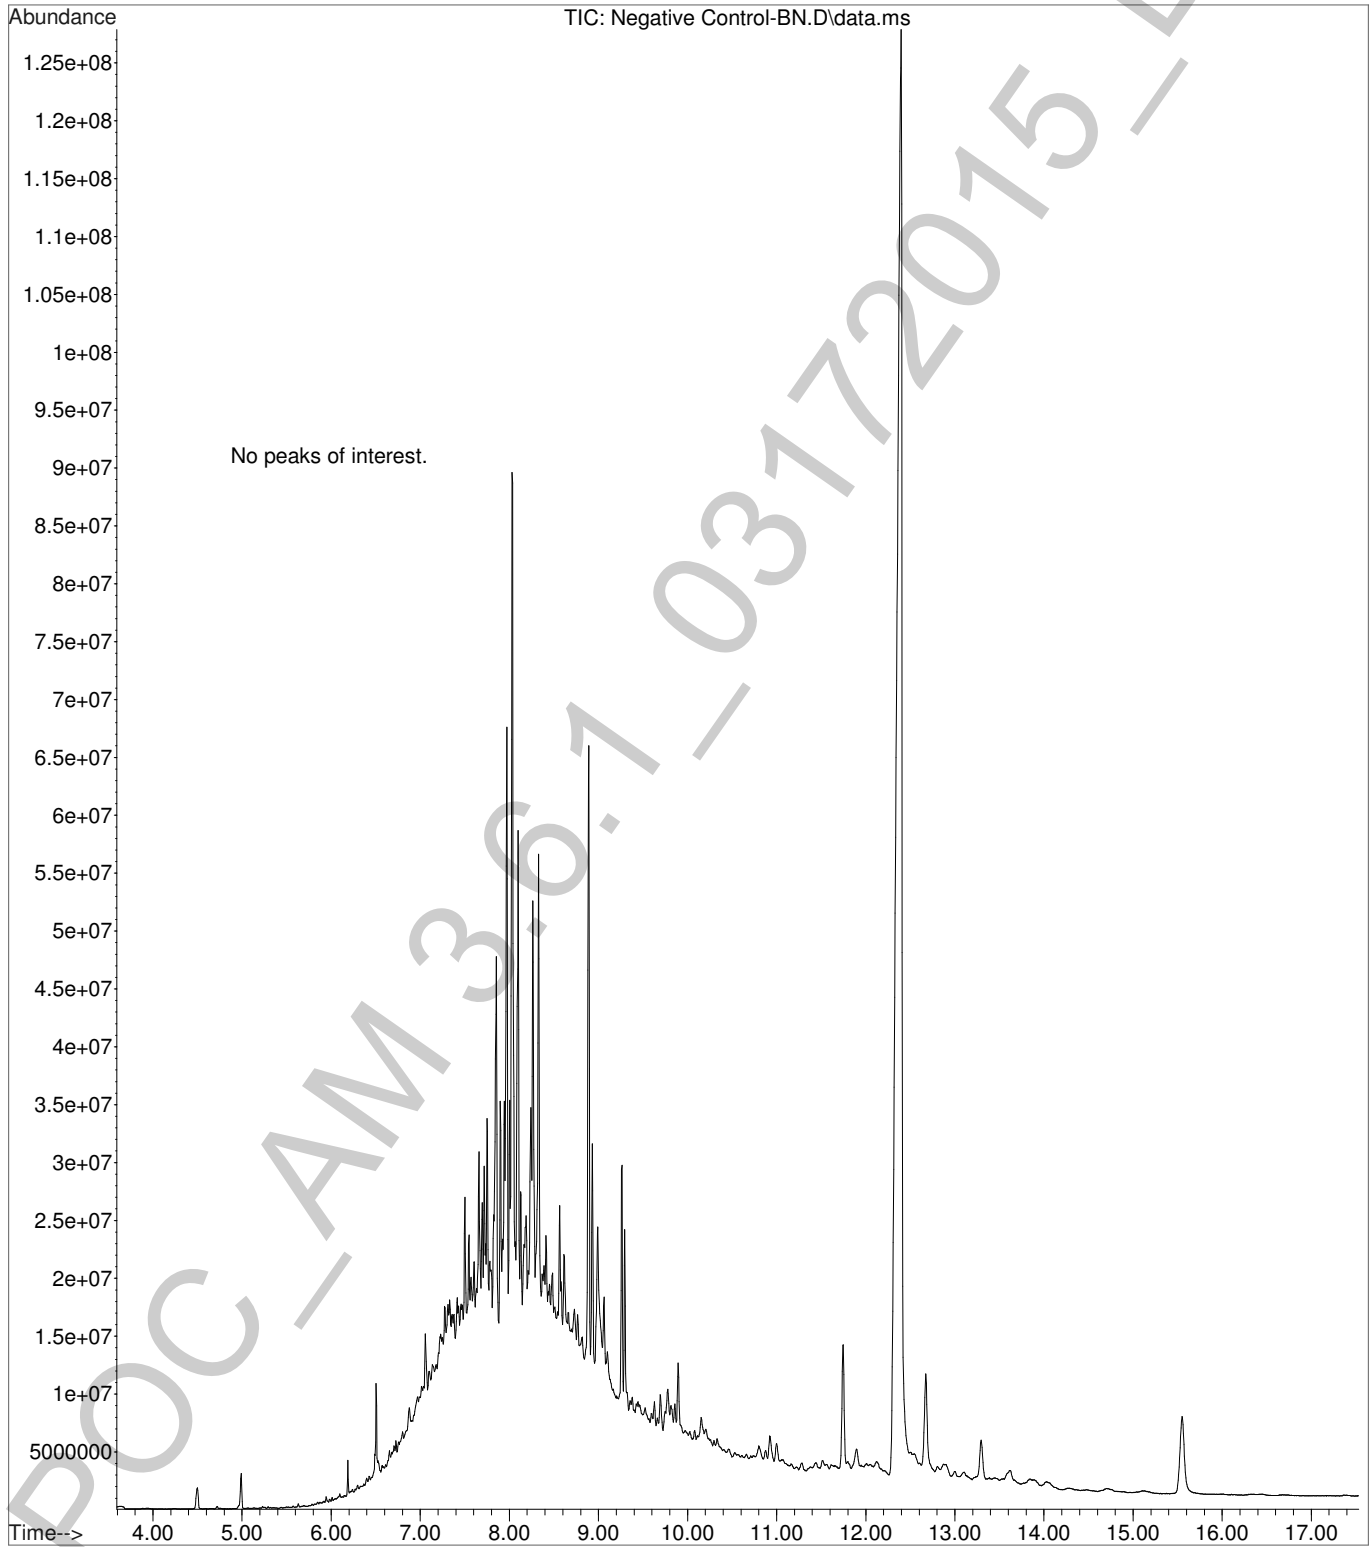


File :C:\gcms\1\data\Blood\031715BN\Negative Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 17 Mar 2015 18:01 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0130
Misc Info : Analytical Method 3.6.1
Vial Number: 1

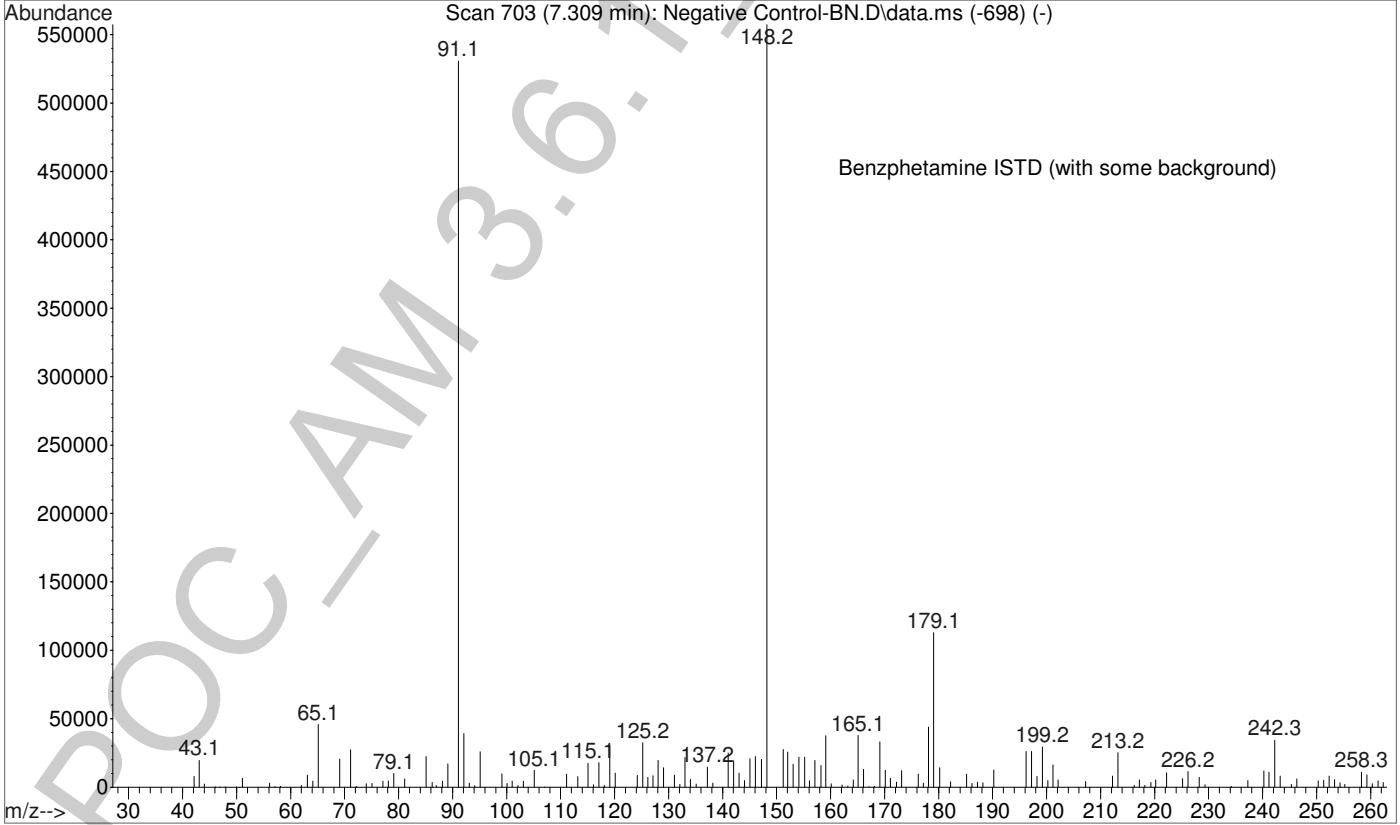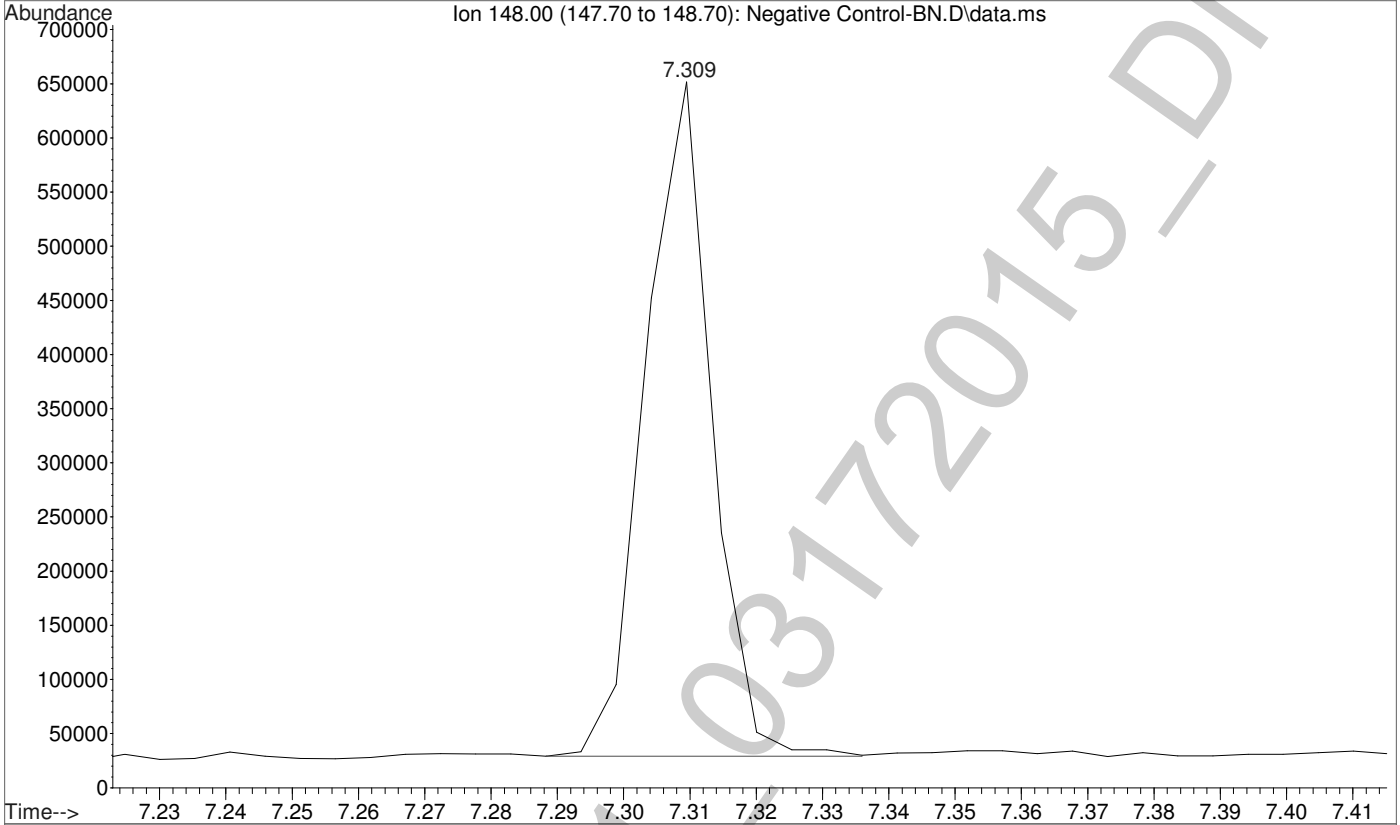



File : C:\gcms\1\data\Blood\031715BN\Negative Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 17 Mar 2015 18:01 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0130
Misc Info : Analytical Method 3.6.1
Vial Number: 1

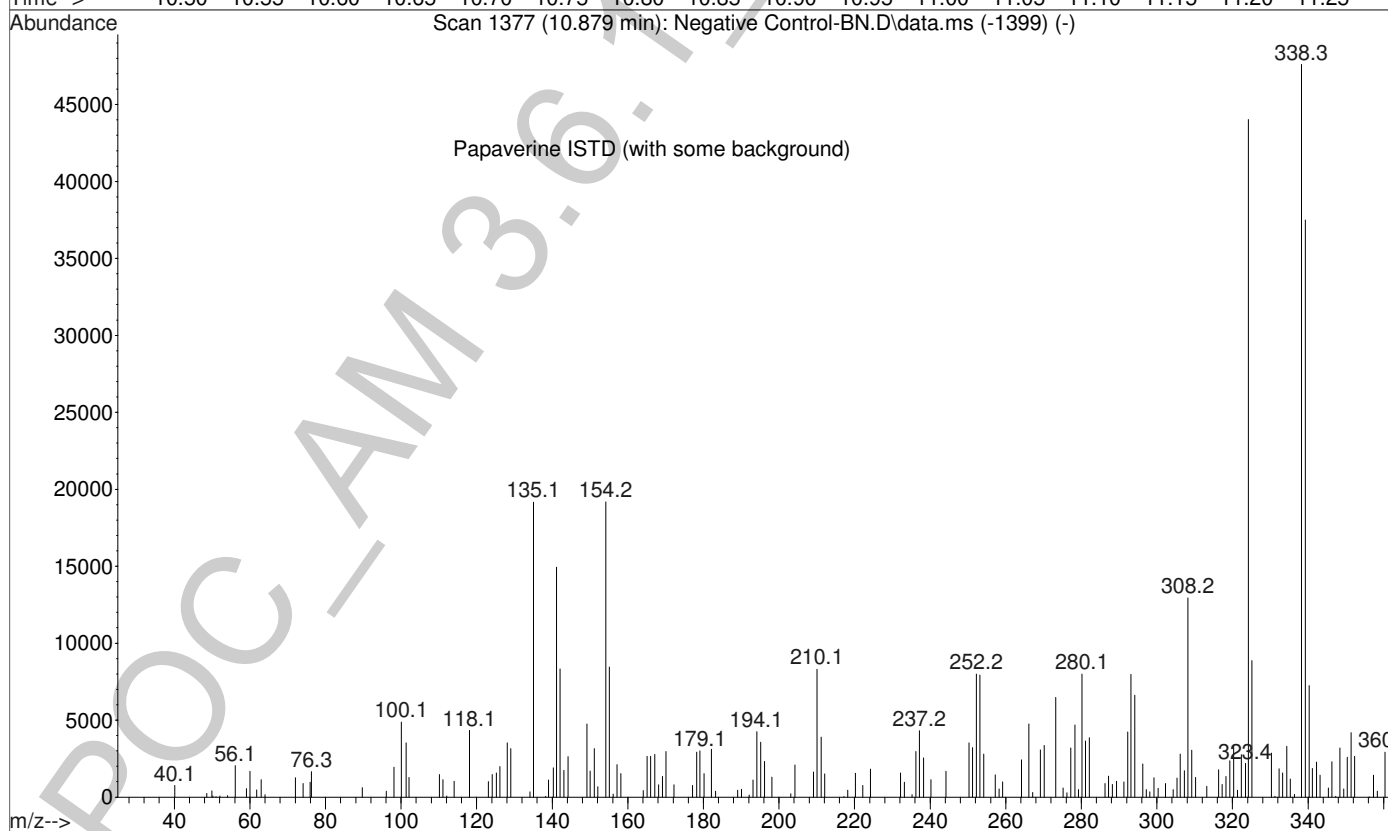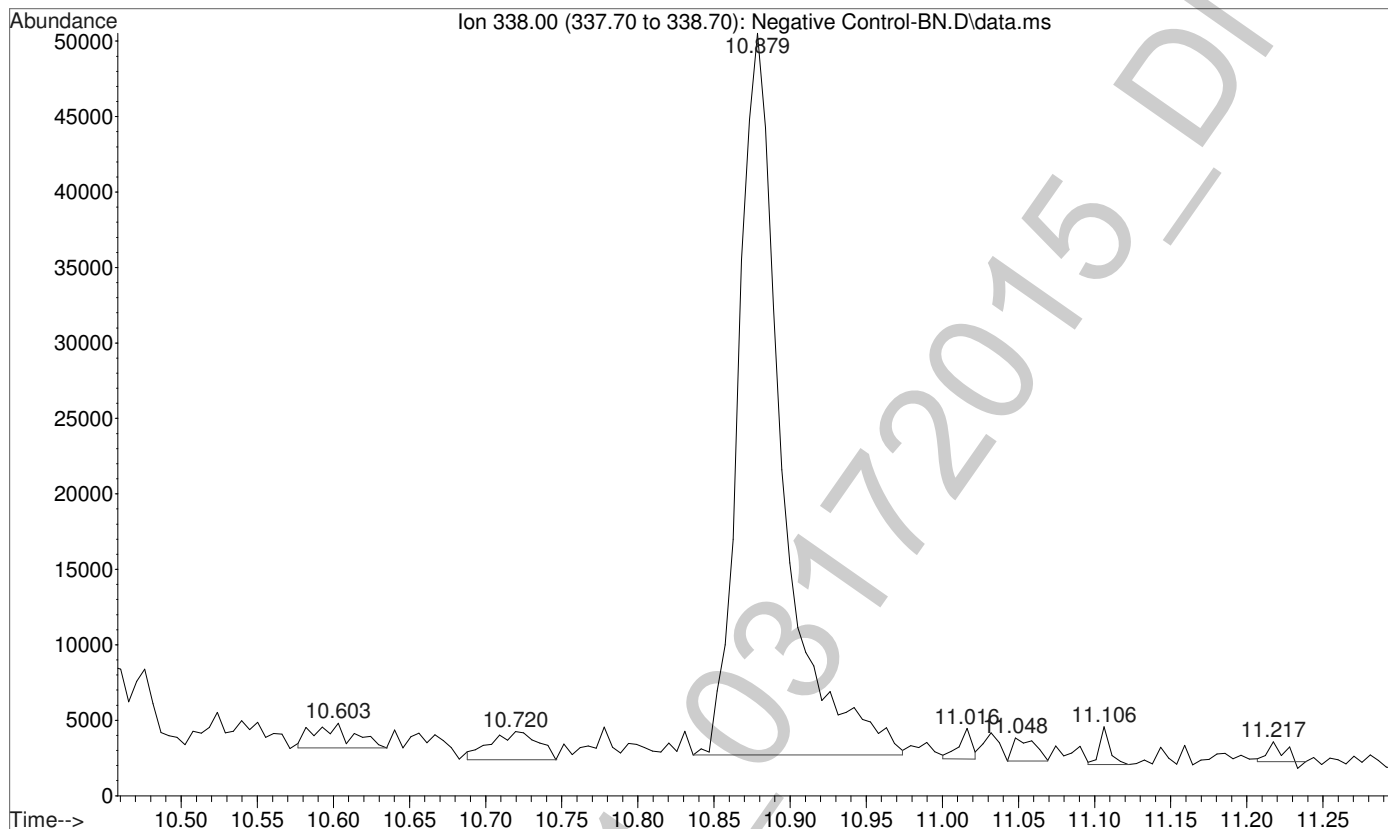



File :C:\gcms\1\data\Blood\031715BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 17 Mar 2015 18:25 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

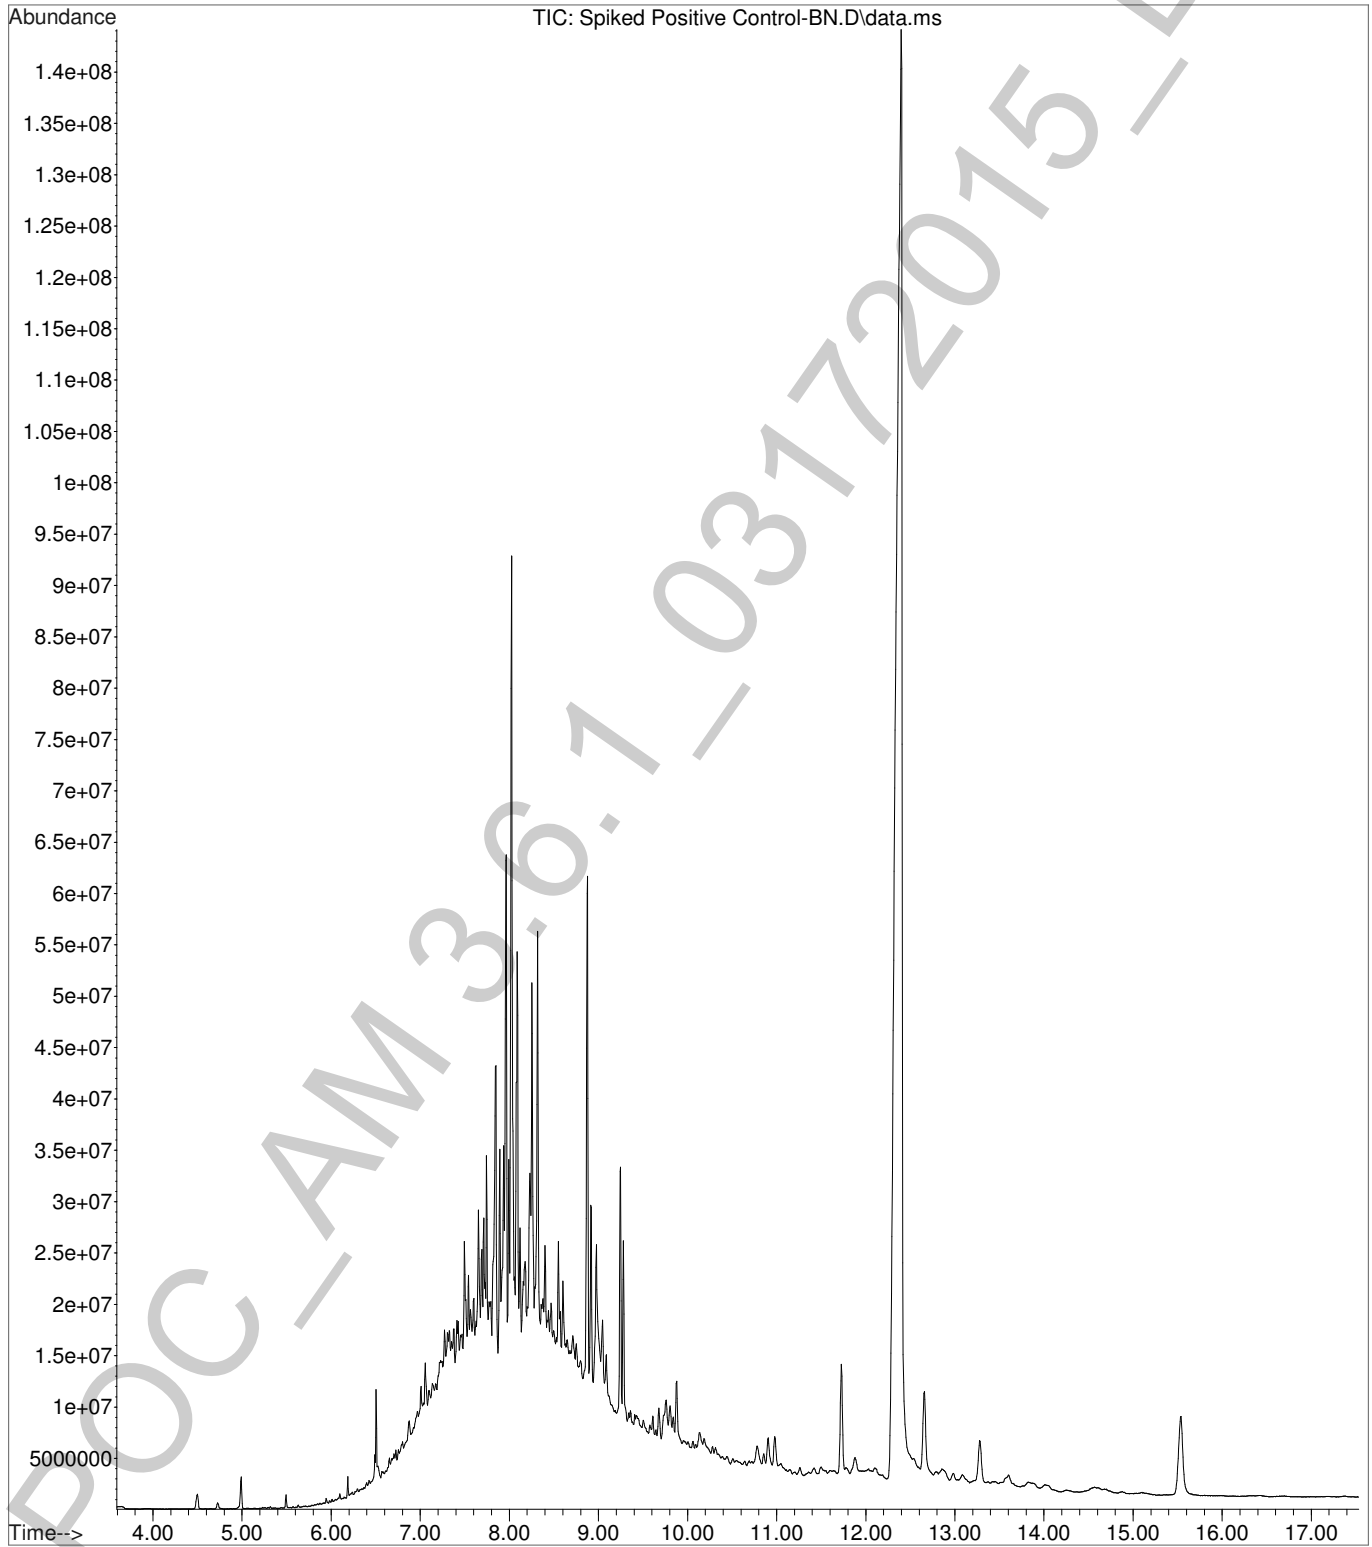



File :C:\gcms\1\data\Blood\031715BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 17 Mar 2015 18:25 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

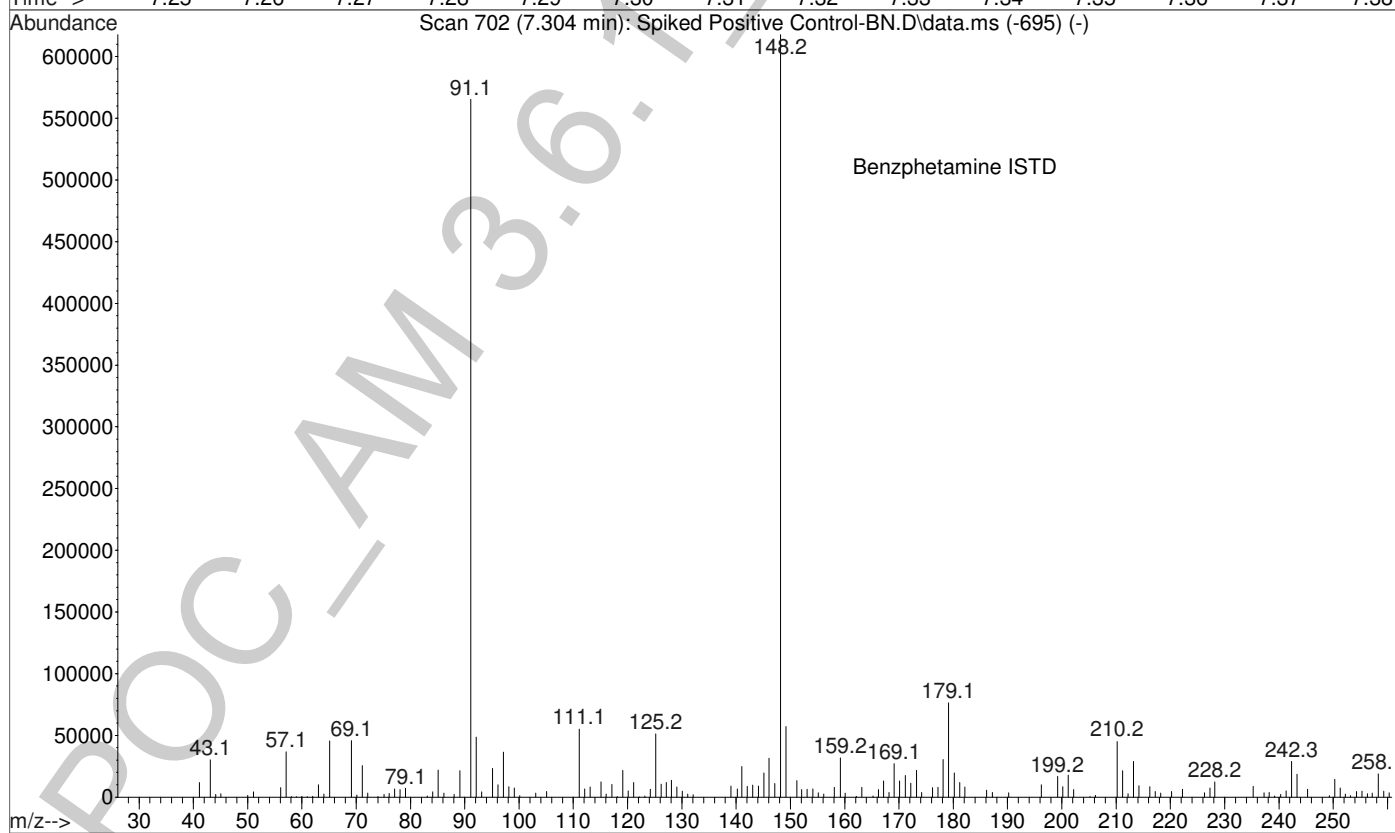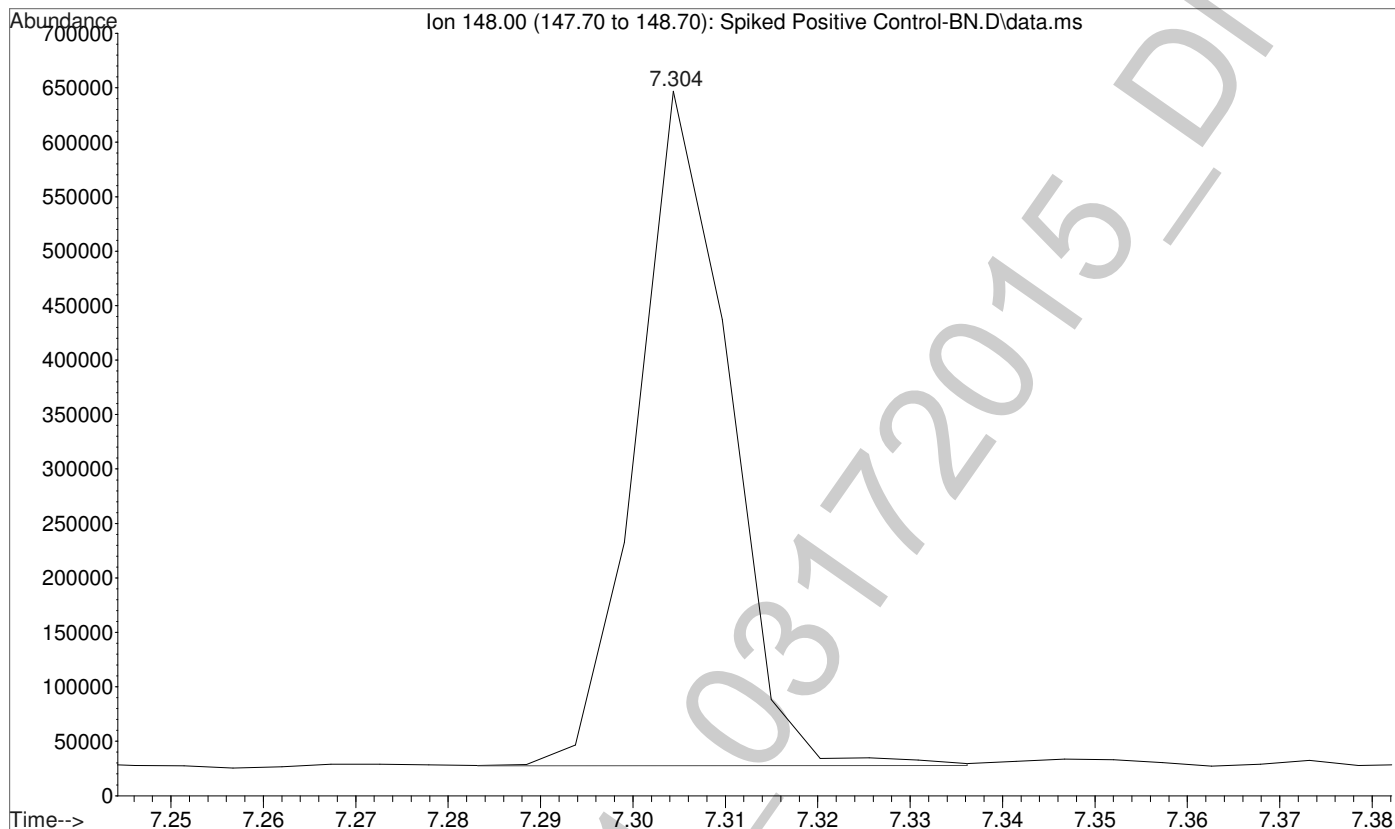



File :C:\gcms\1\data\Blood\031715BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 17 Mar 2015 18:25 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

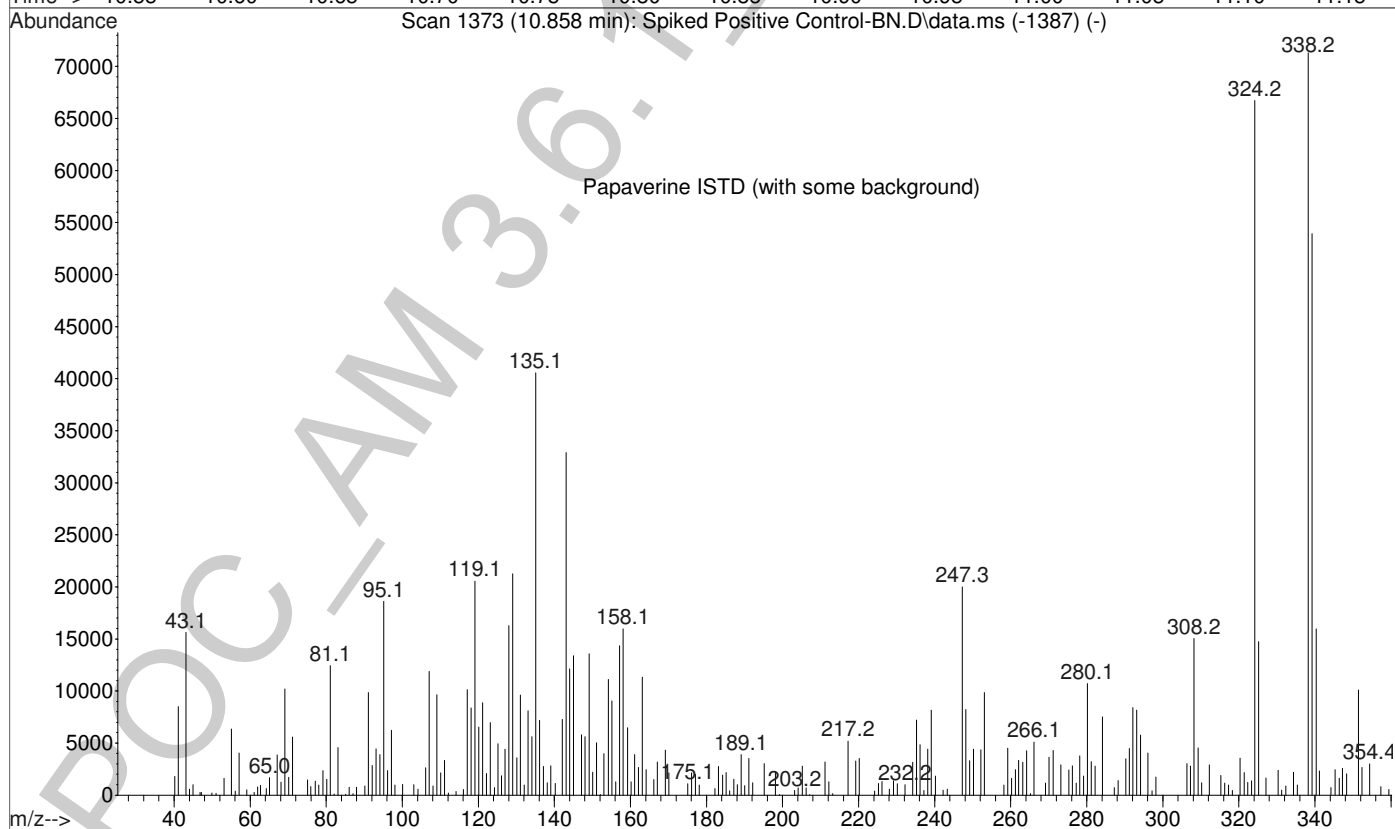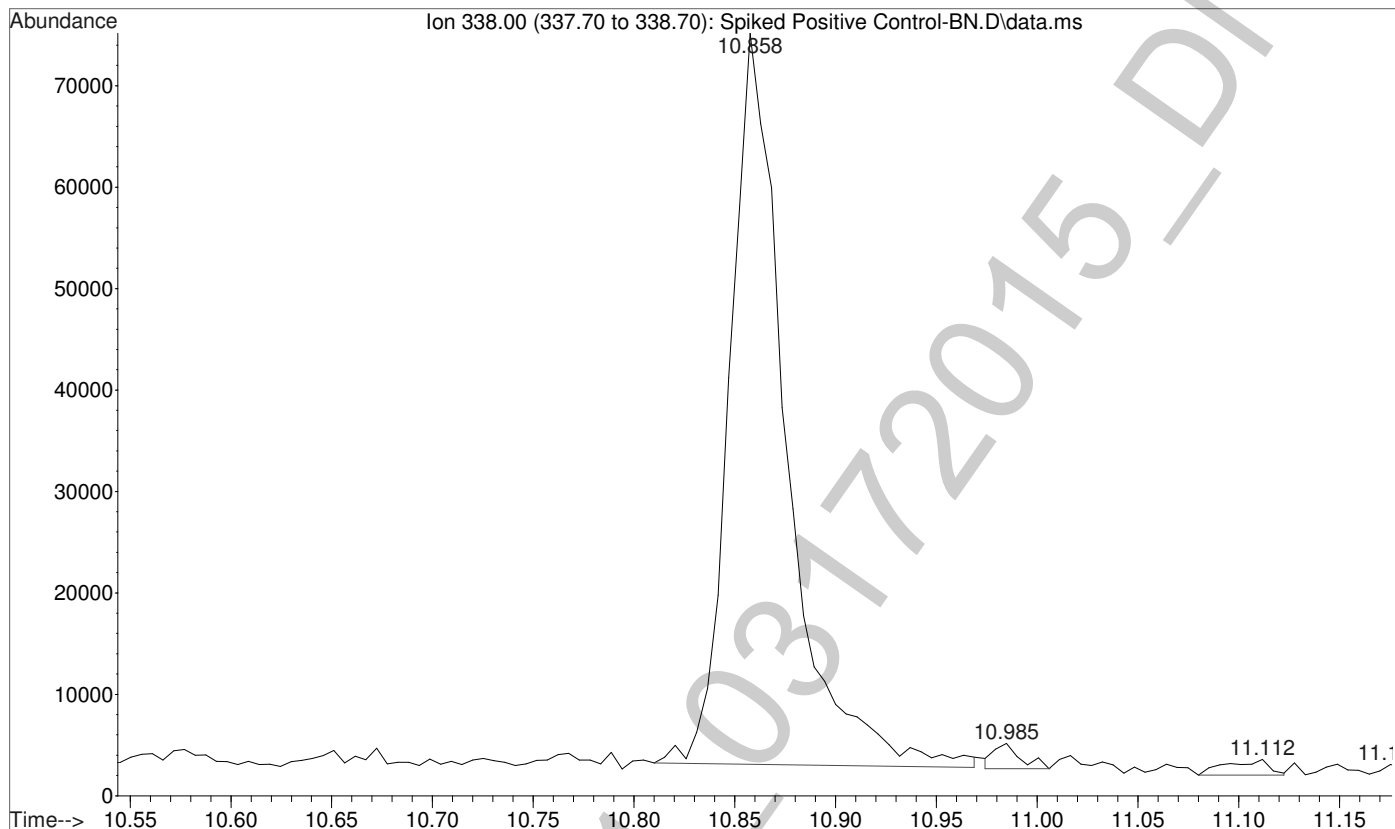



File :C:\gcms\1\data\Blood\031715BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 17 Mar 2015 18:25 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

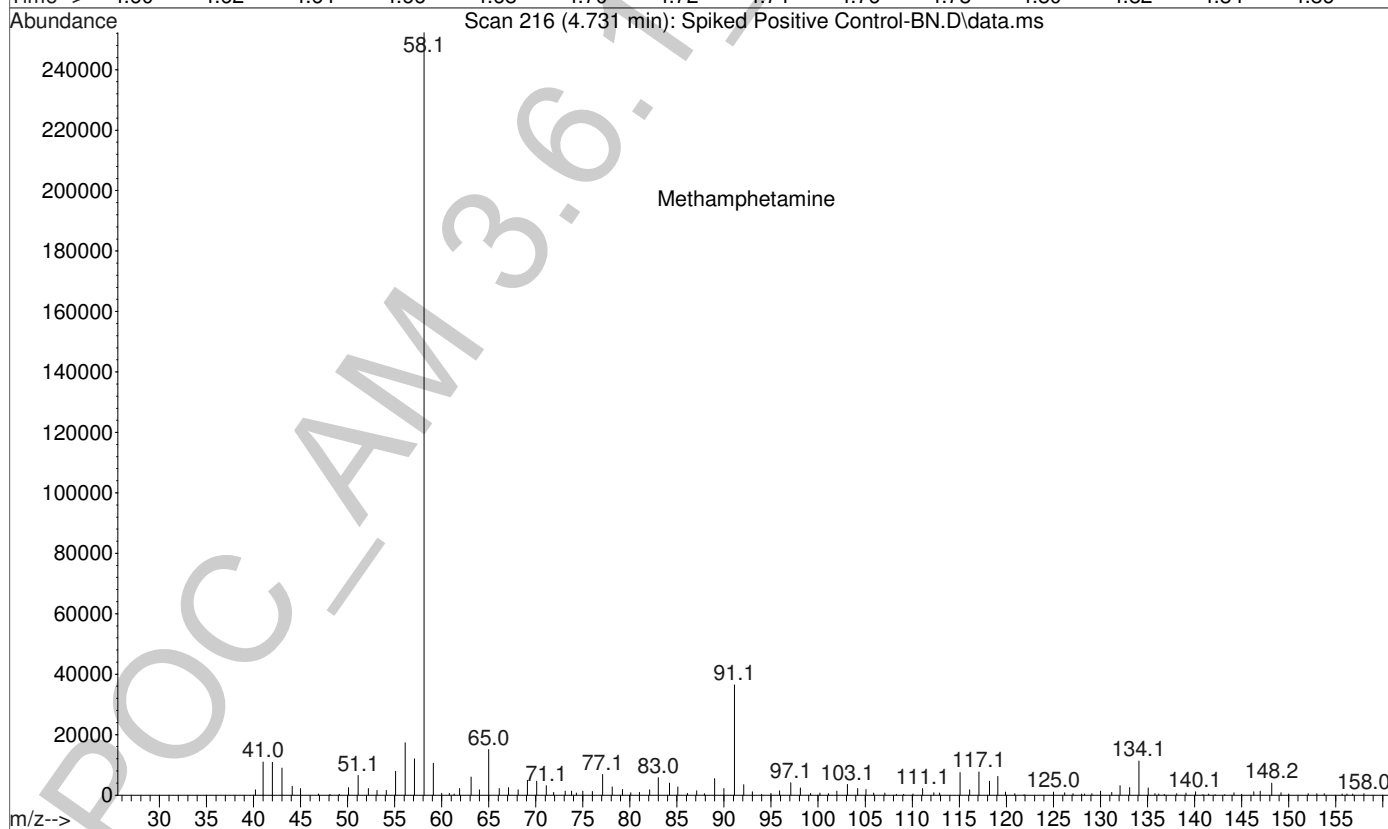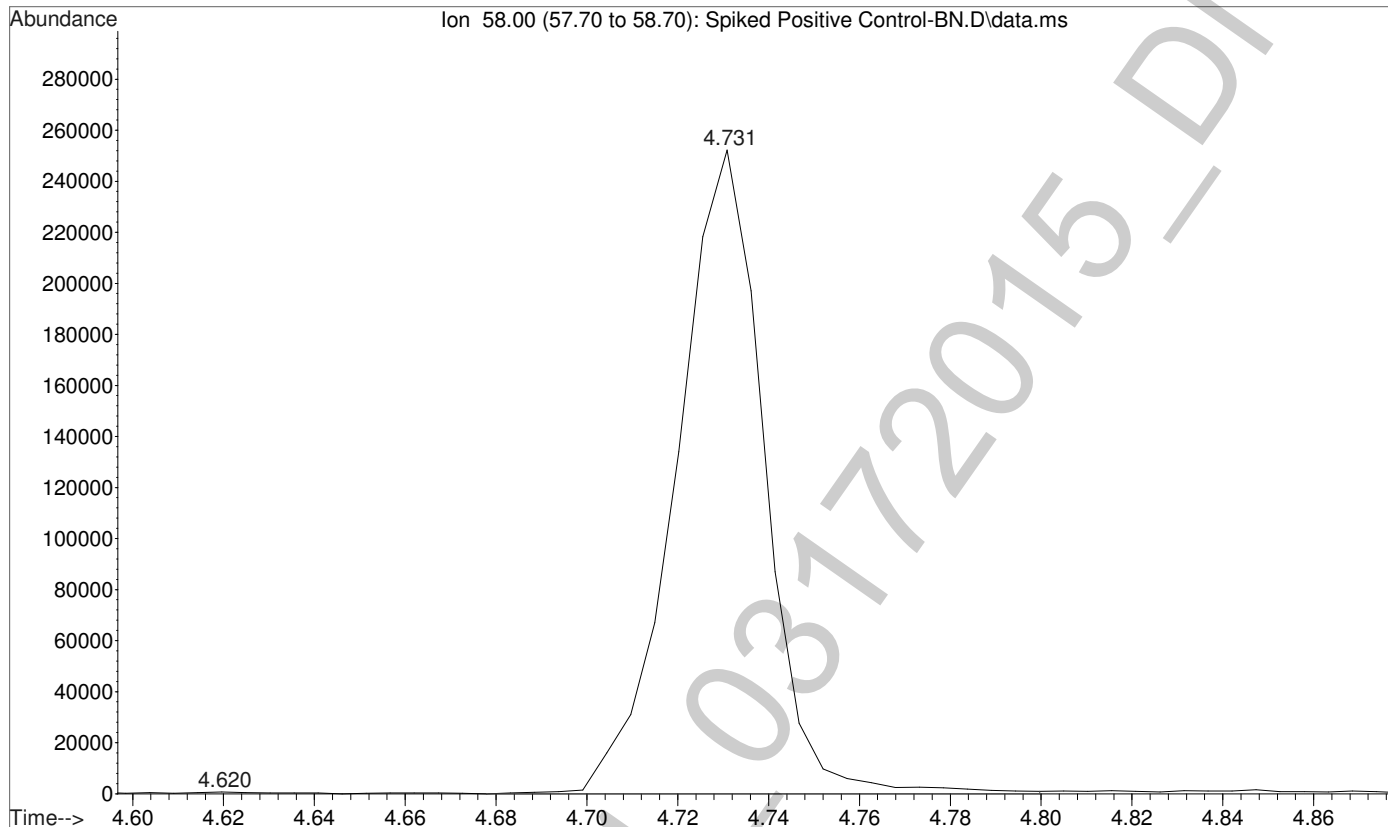



File :C:\gcms\1\data\Blood\031715BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 17 Mar 2015 18:25 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

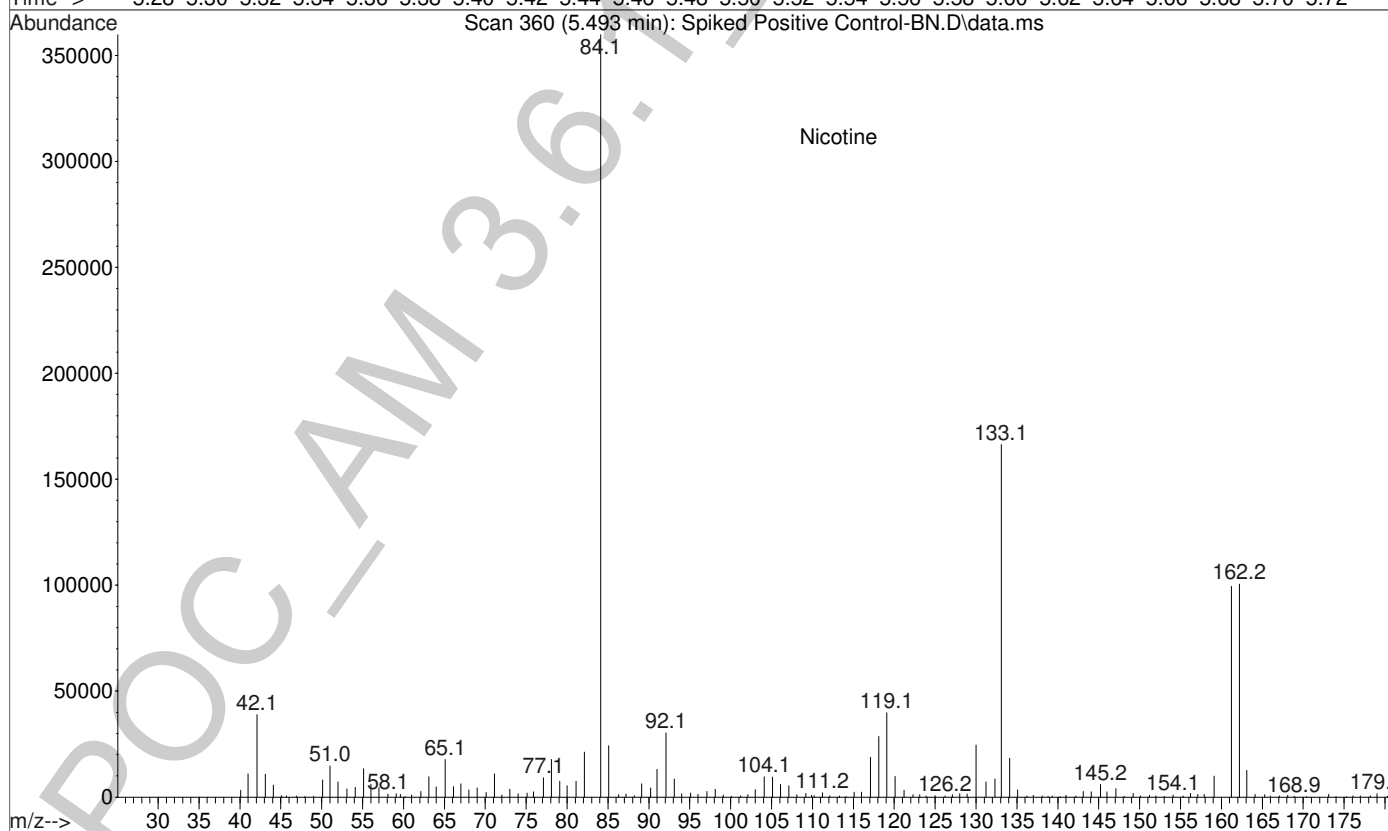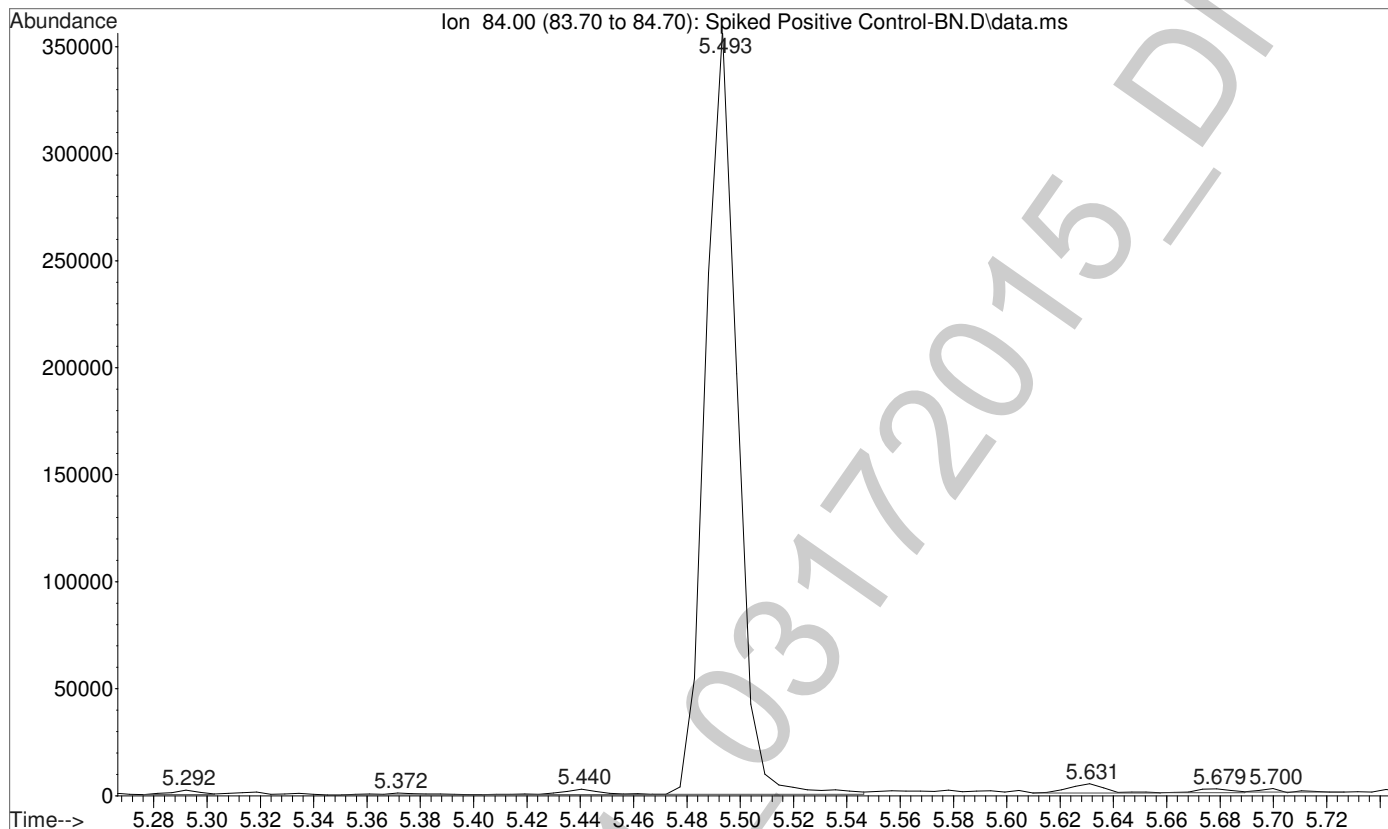



File :C:\gcms\1\data\Blood\031715BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 17 Mar 2015 18:25 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

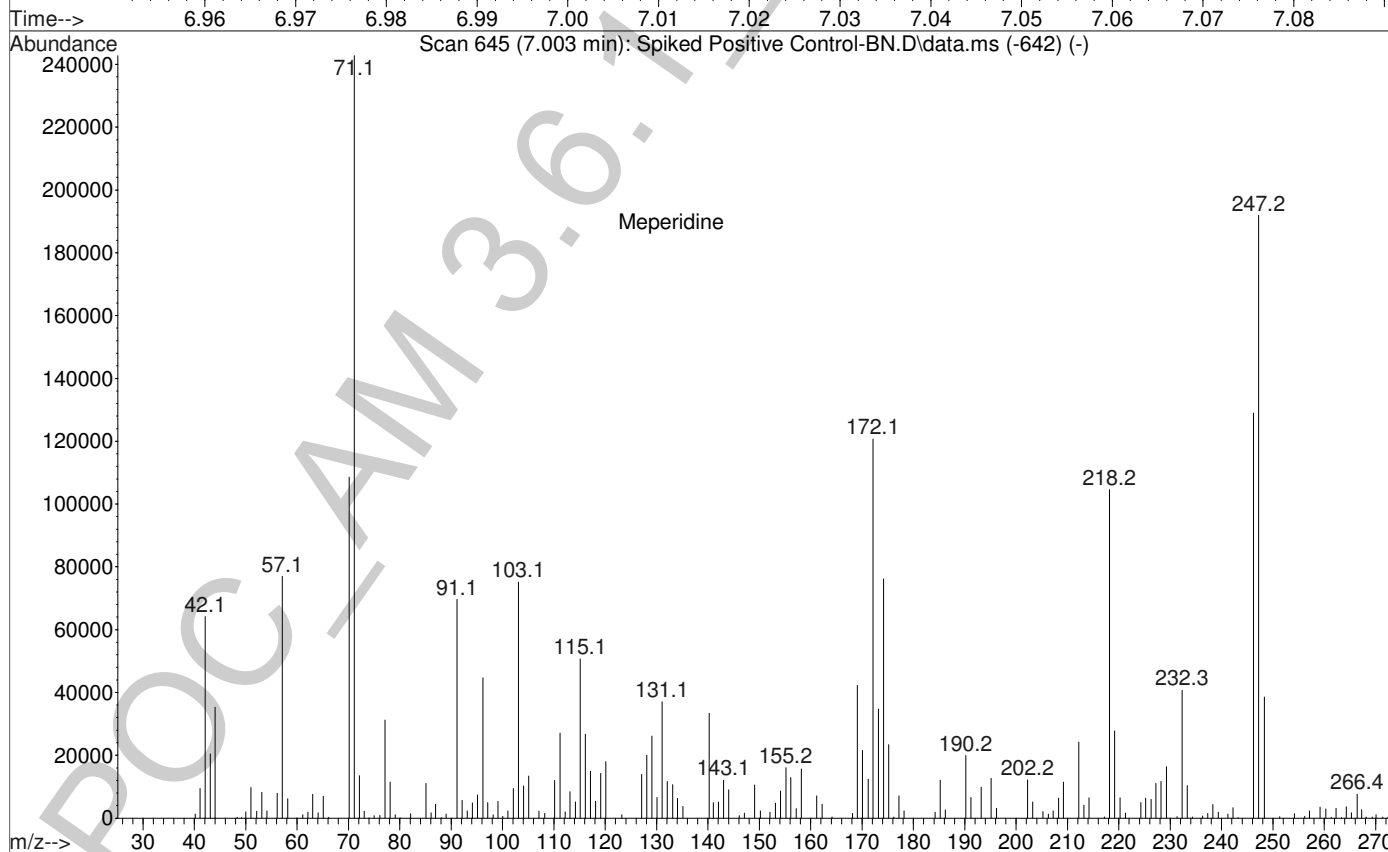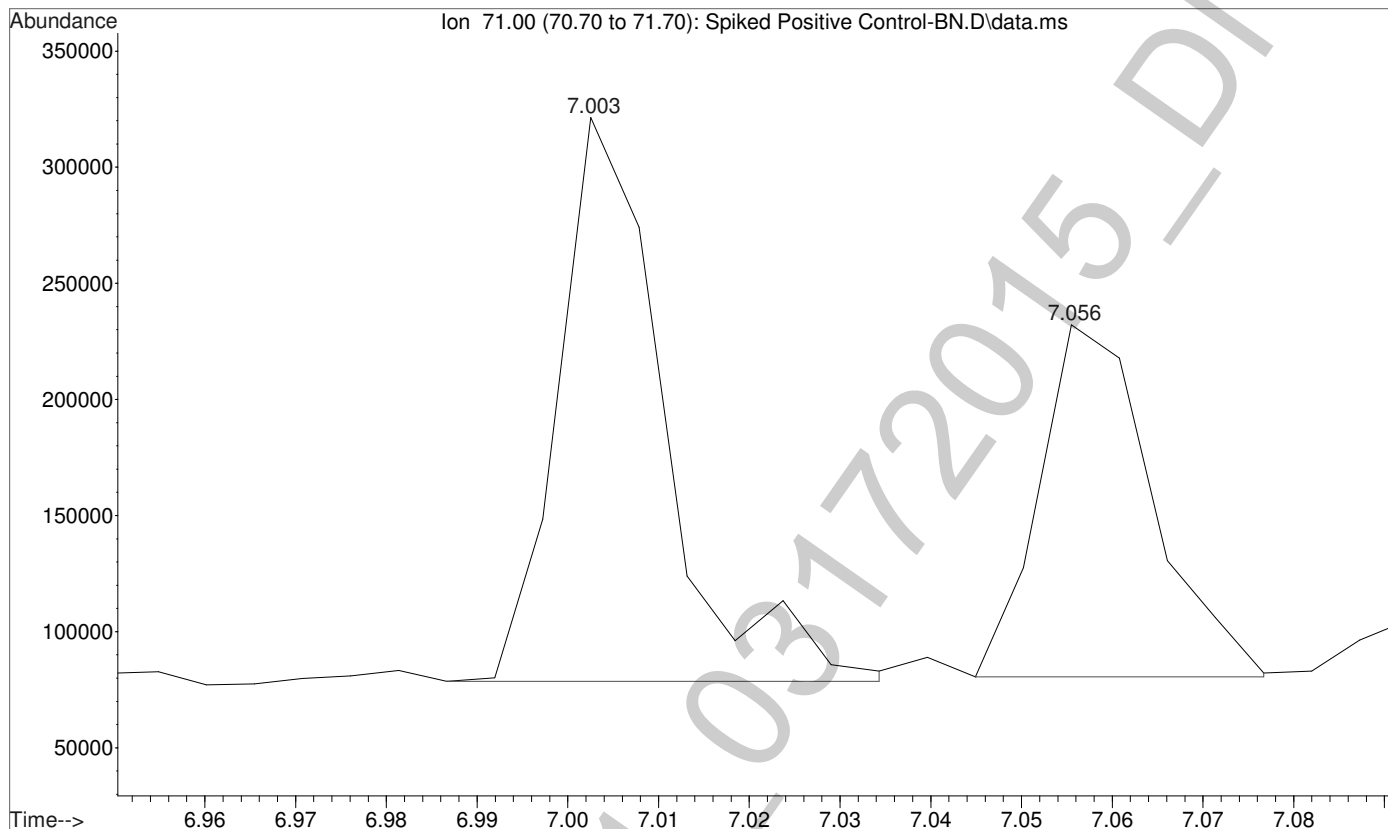



File :C:\gcms\1\data\Blood\031715BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 17 Mar 2015 18:25 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

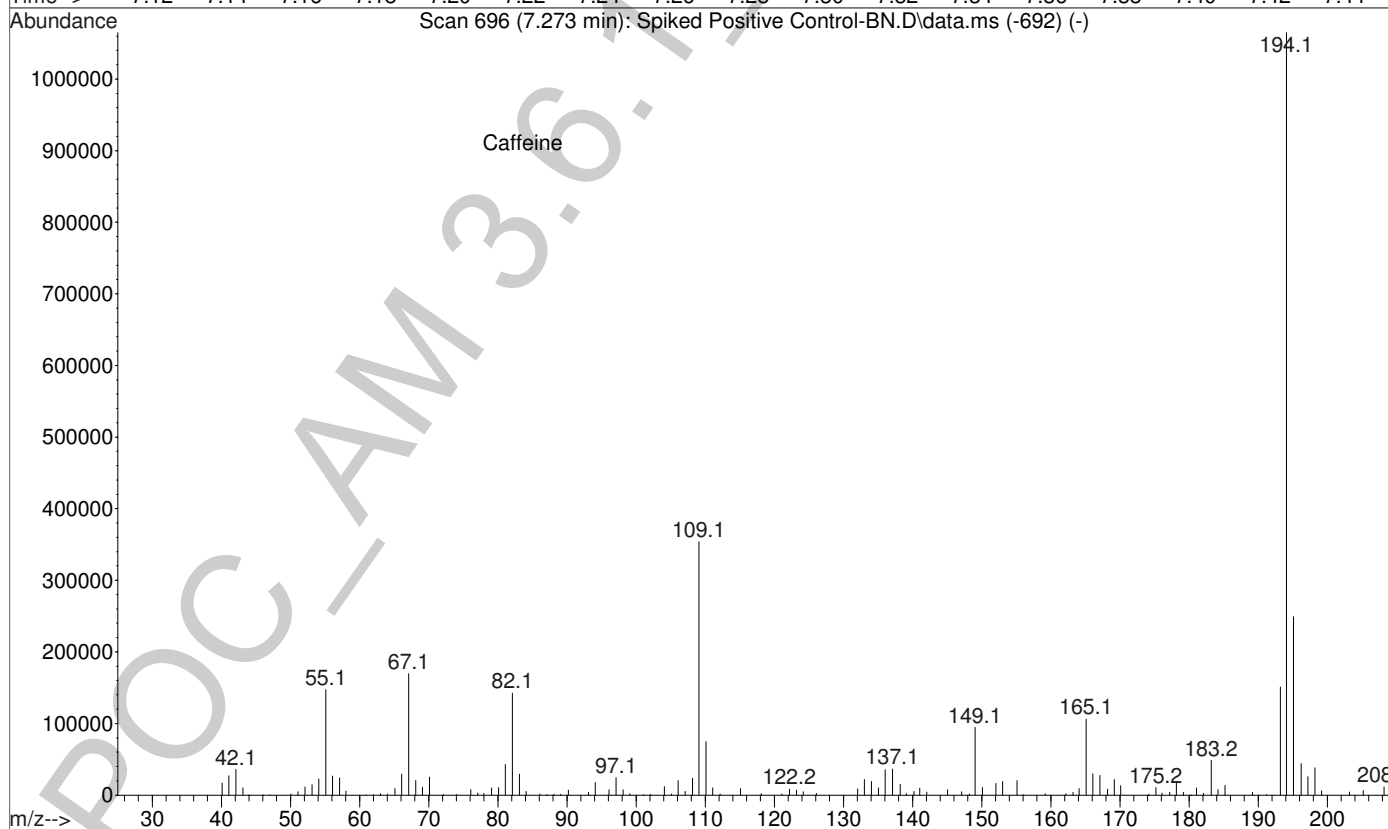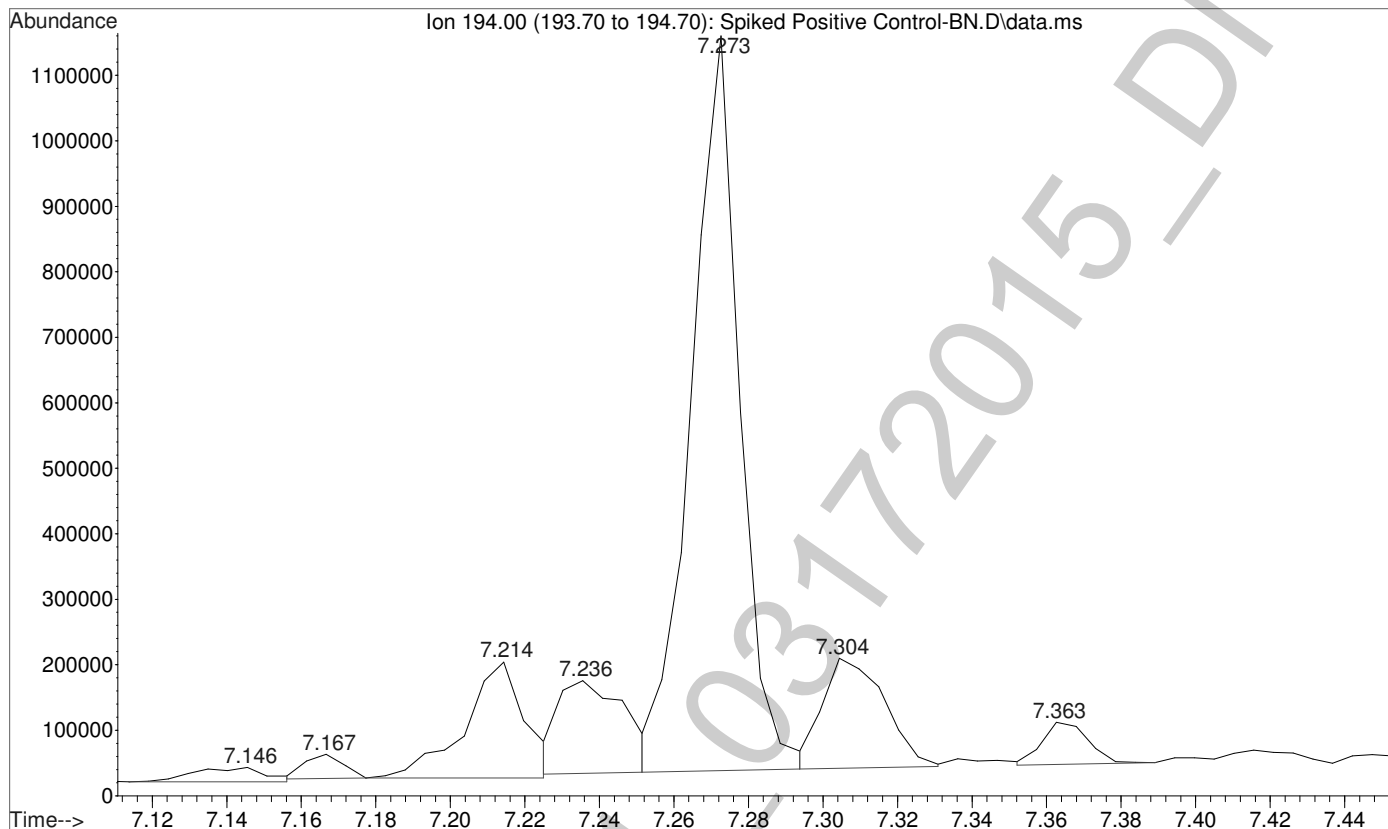



File :C:\gcms\1\data\Blood\031715BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 17 Mar 2015 18:25 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

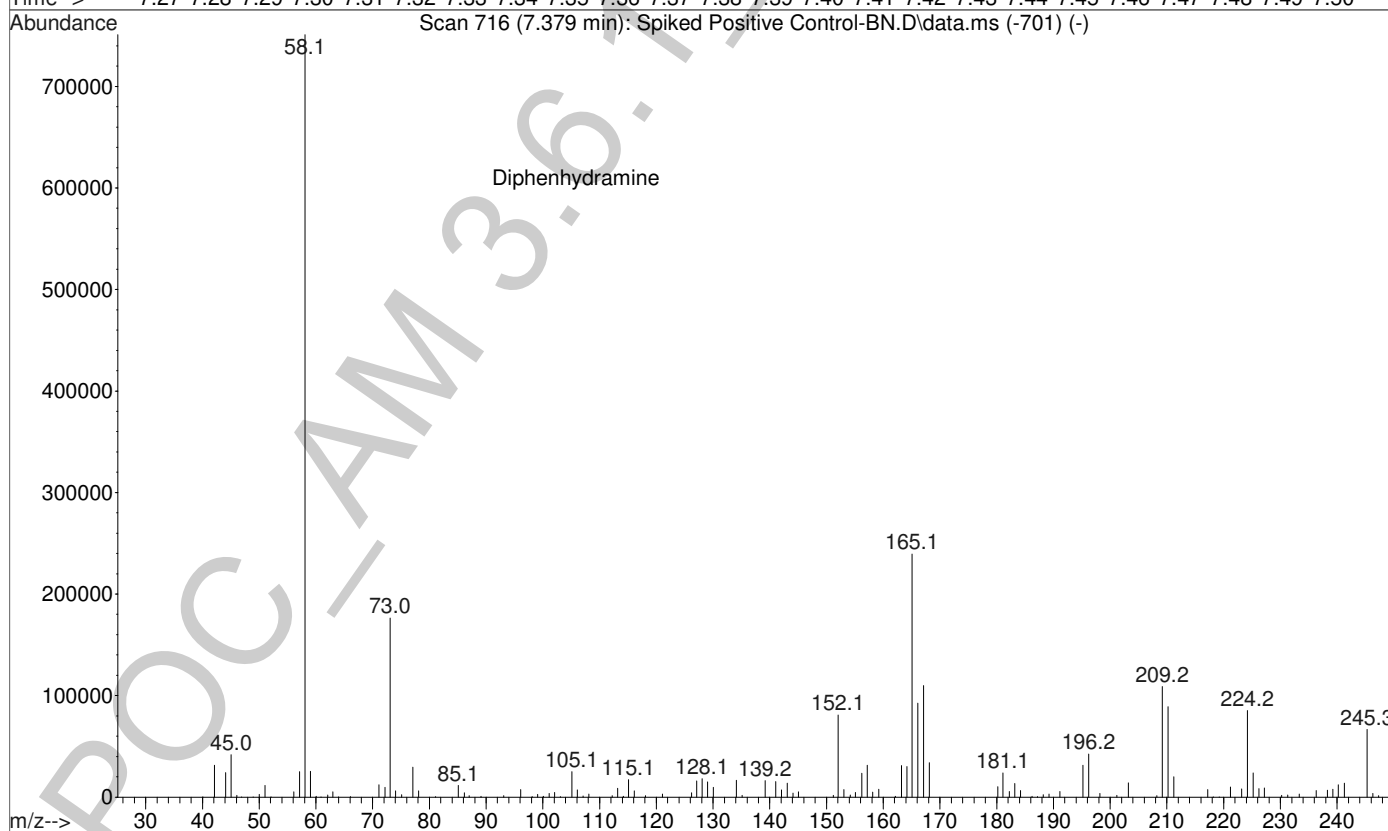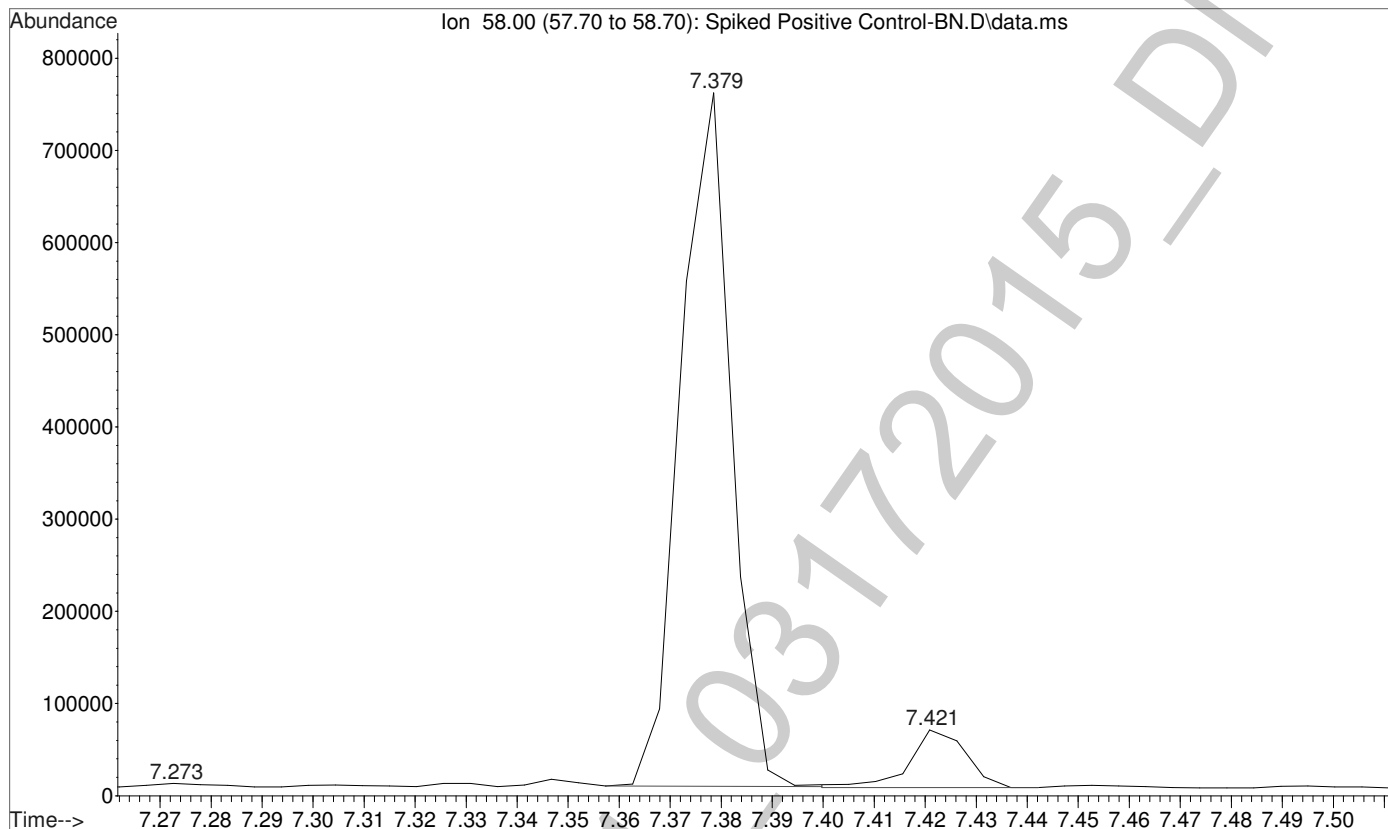



File :C:\gcms\1\data\Blood\031715BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 17 Mar 2015 18:25 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

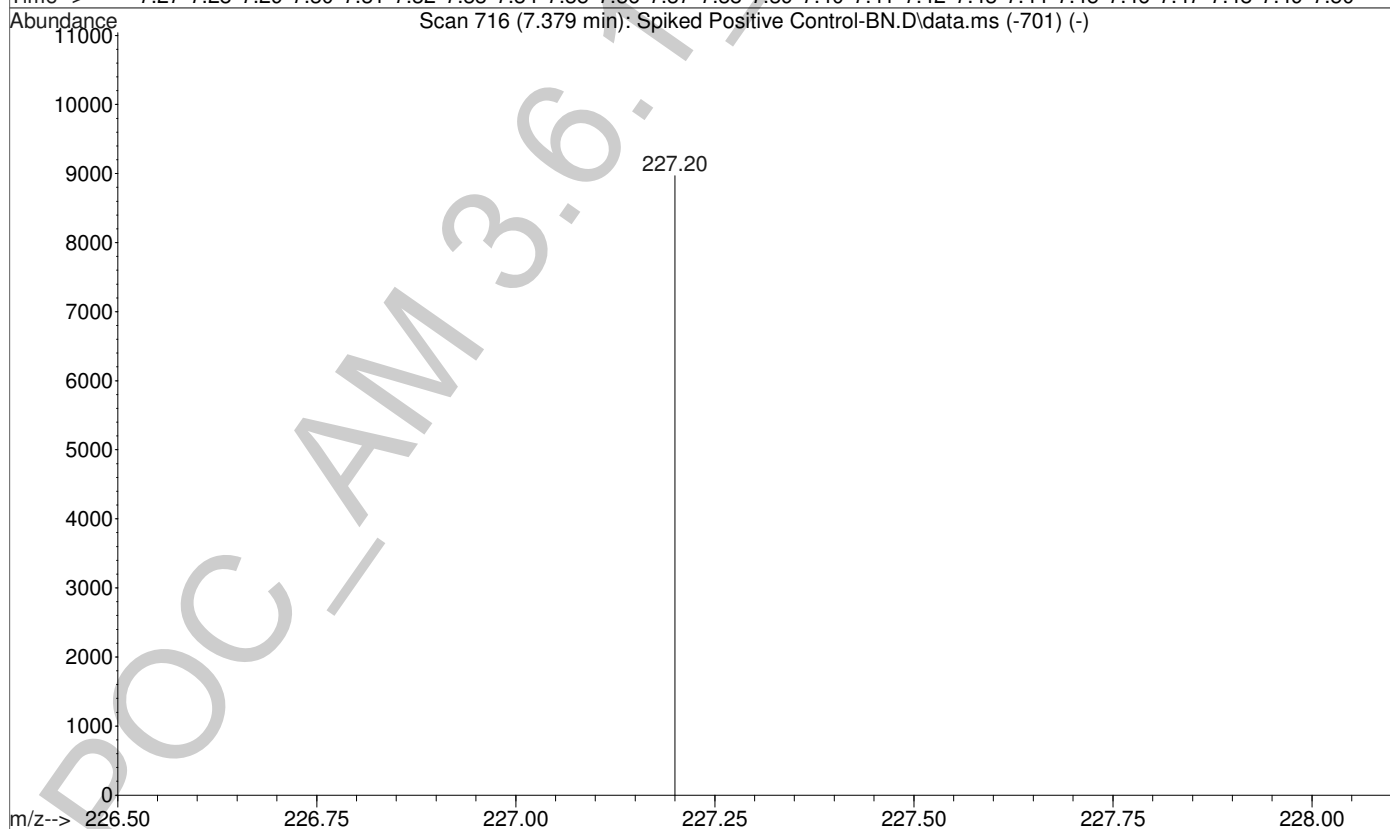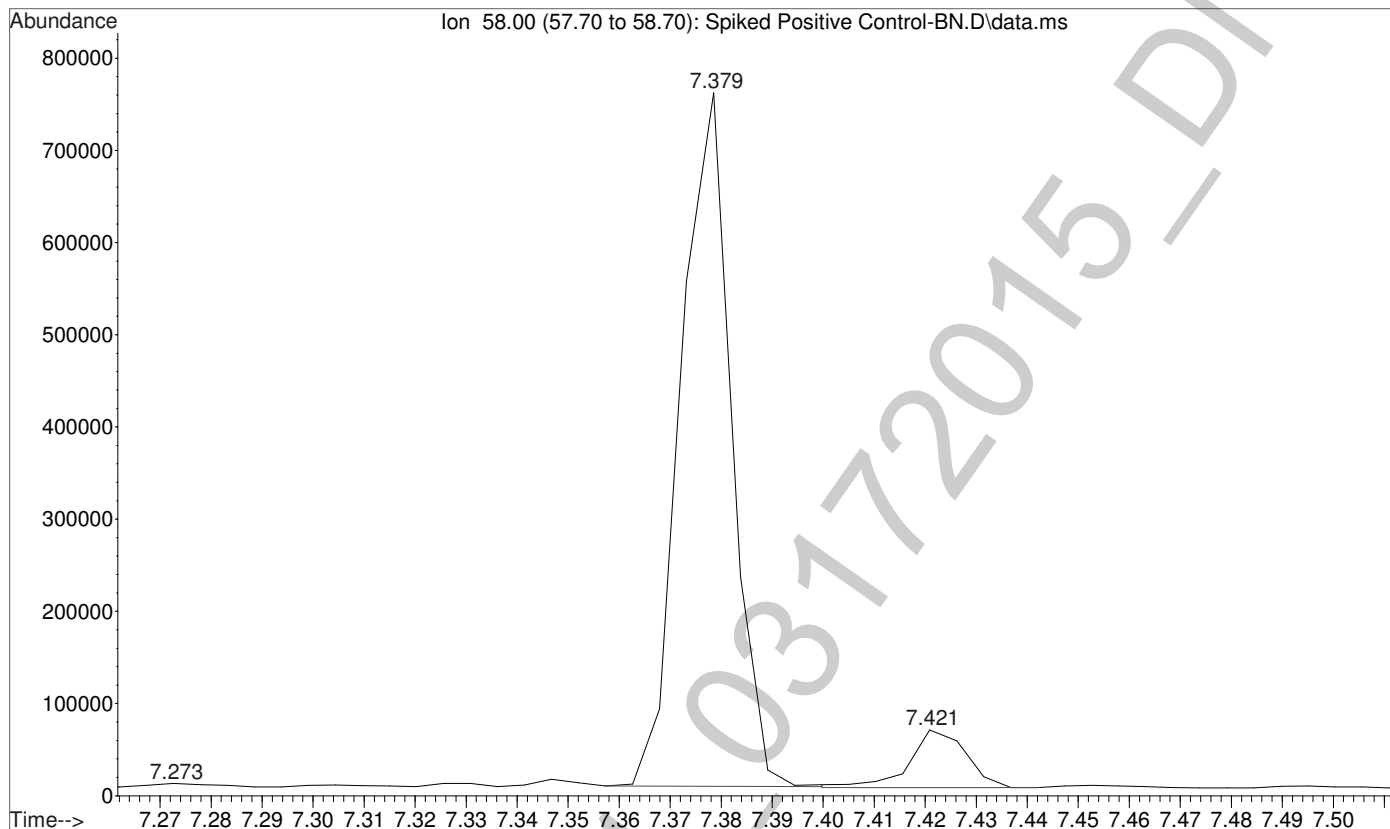



File :C:\gcms\1\data\Blood\031715BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 17 Mar 2015 18:25 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

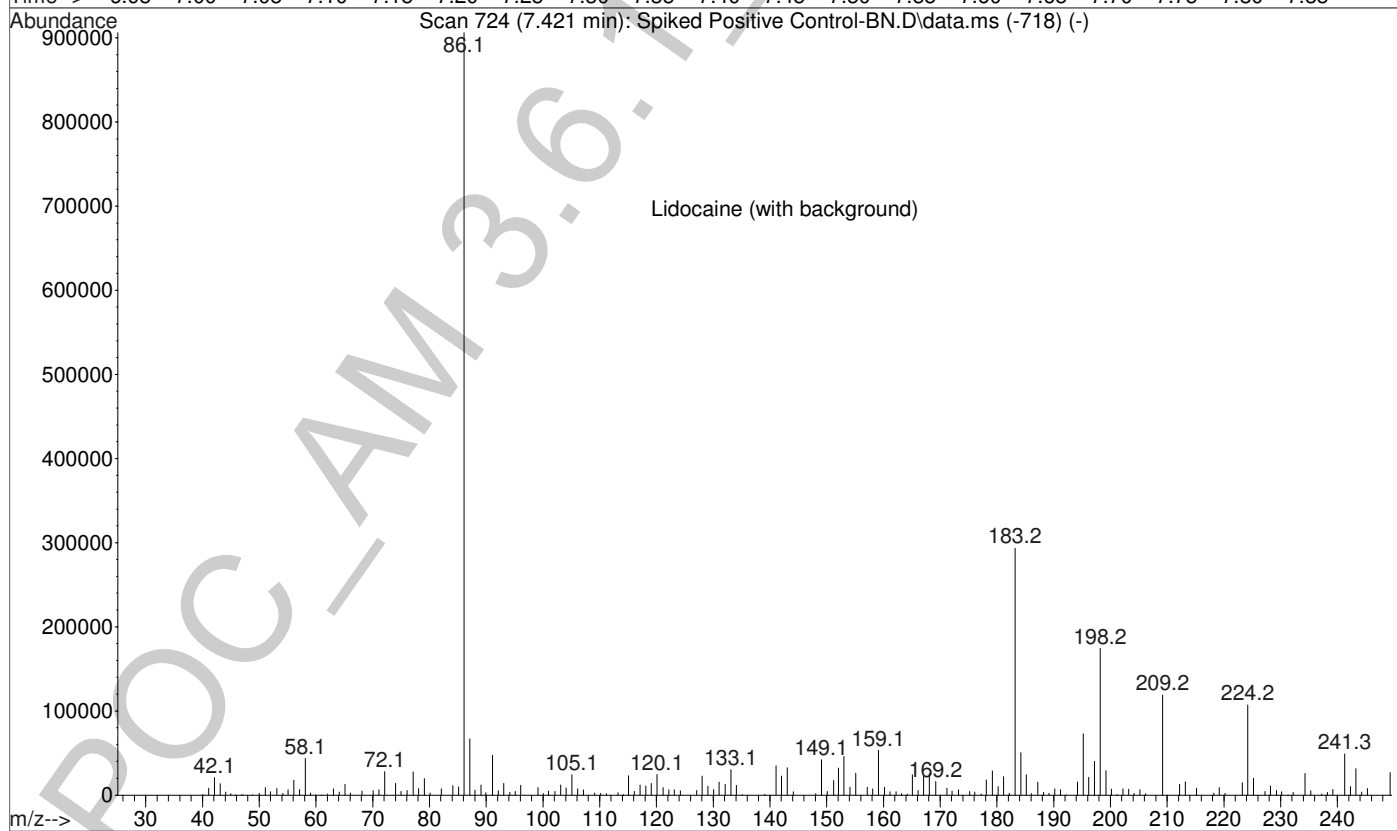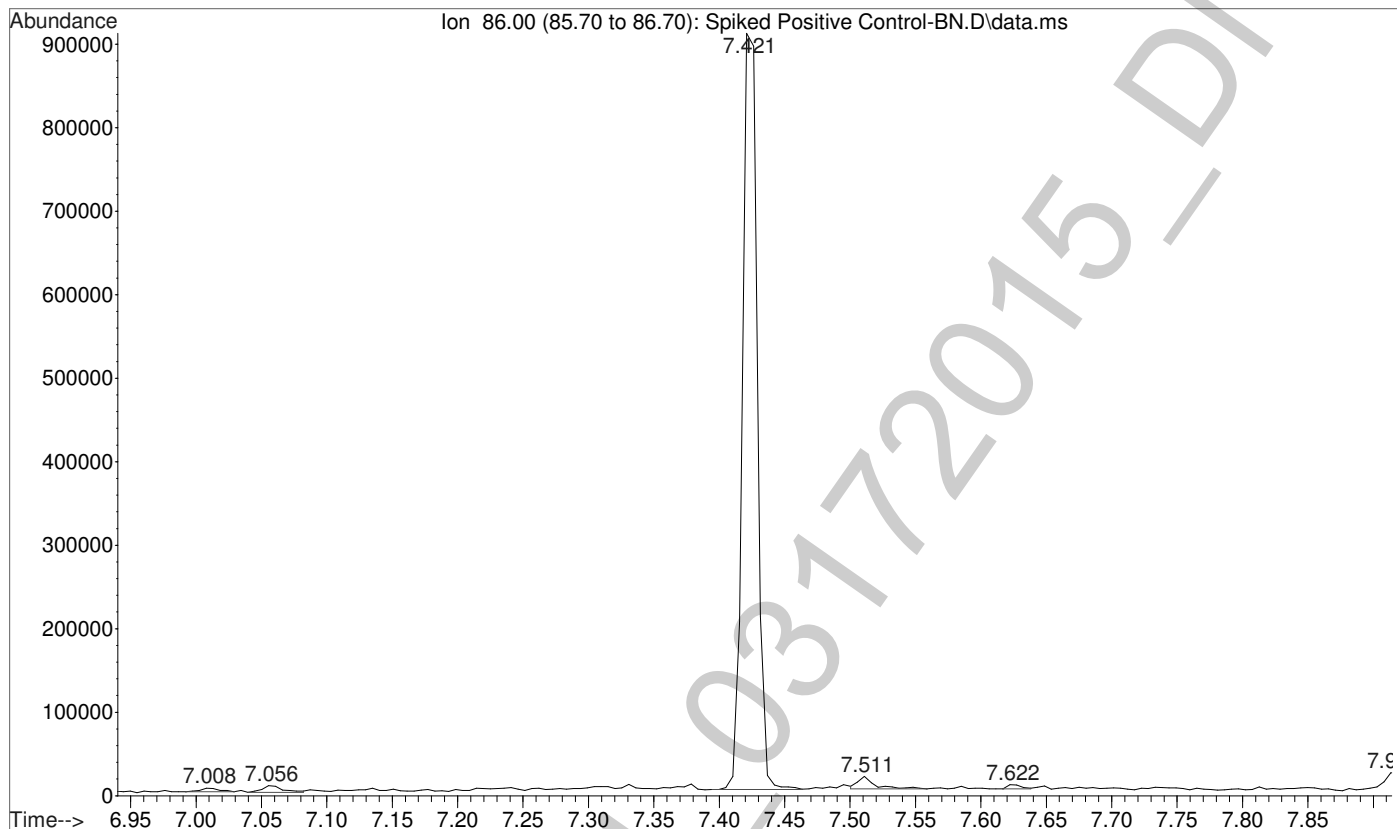



File :C:\gcms\1\data\Blood\031715BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 17 Mar 2015 18:25 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

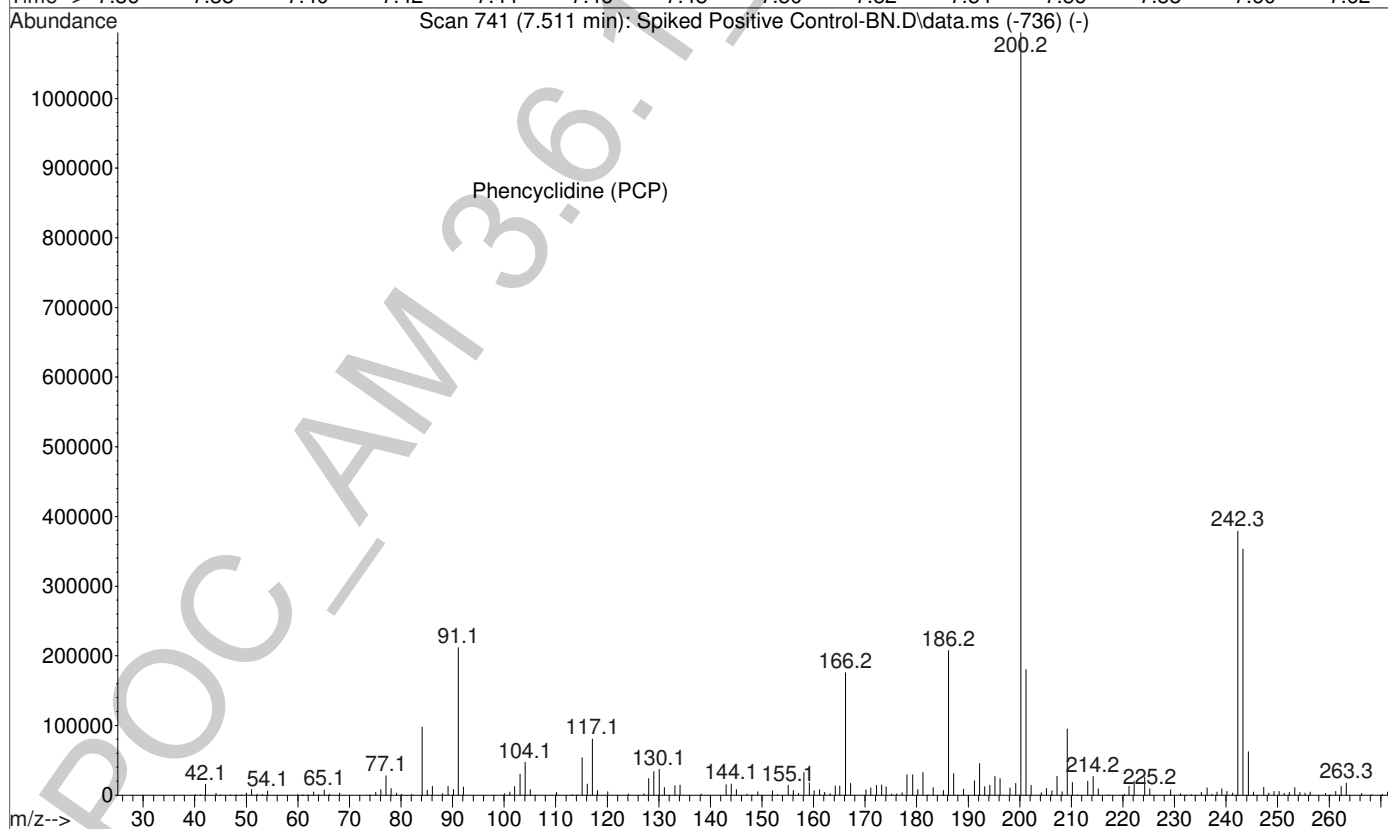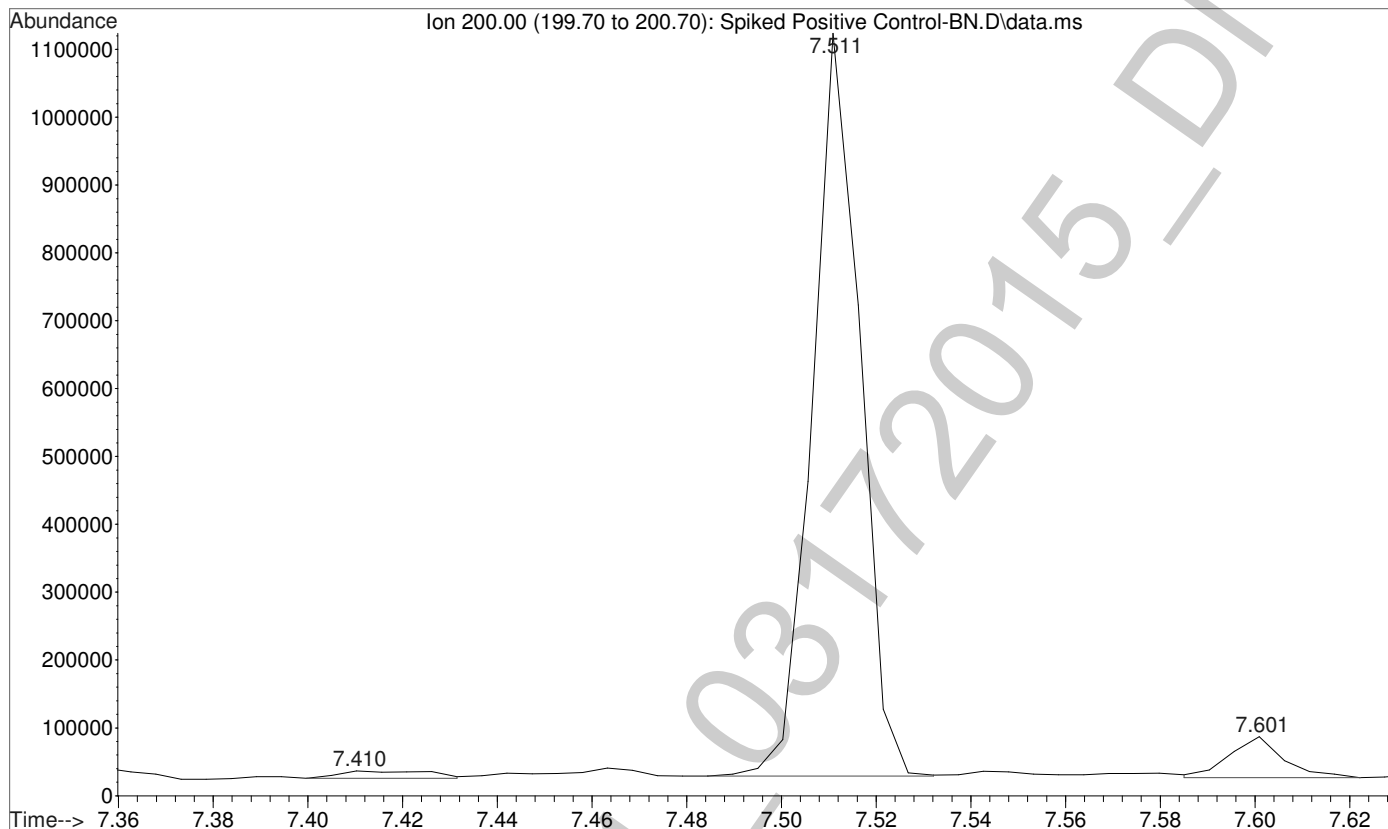



File :C:\gcms\1\data\Blood\031715BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 17 Mar 2015 18:25 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

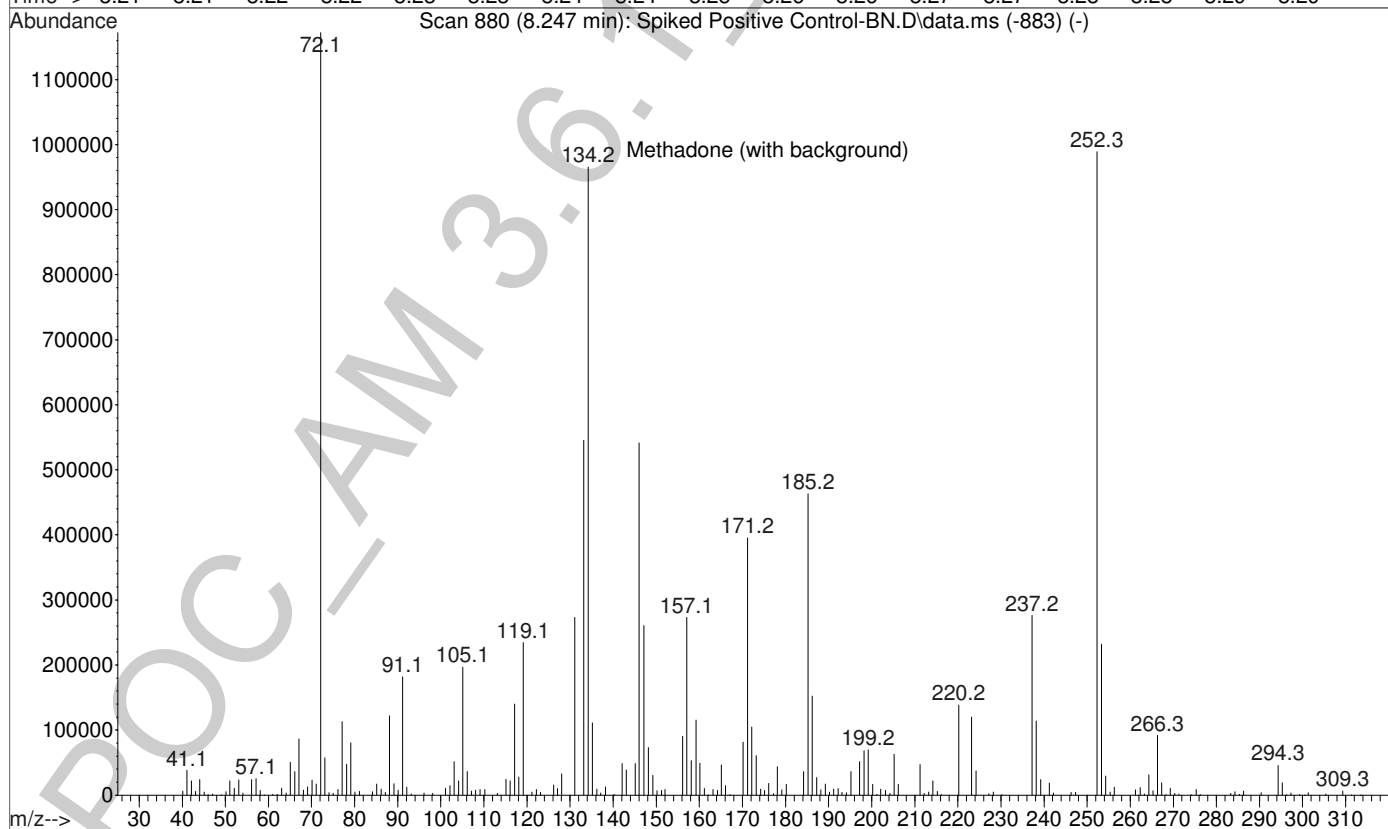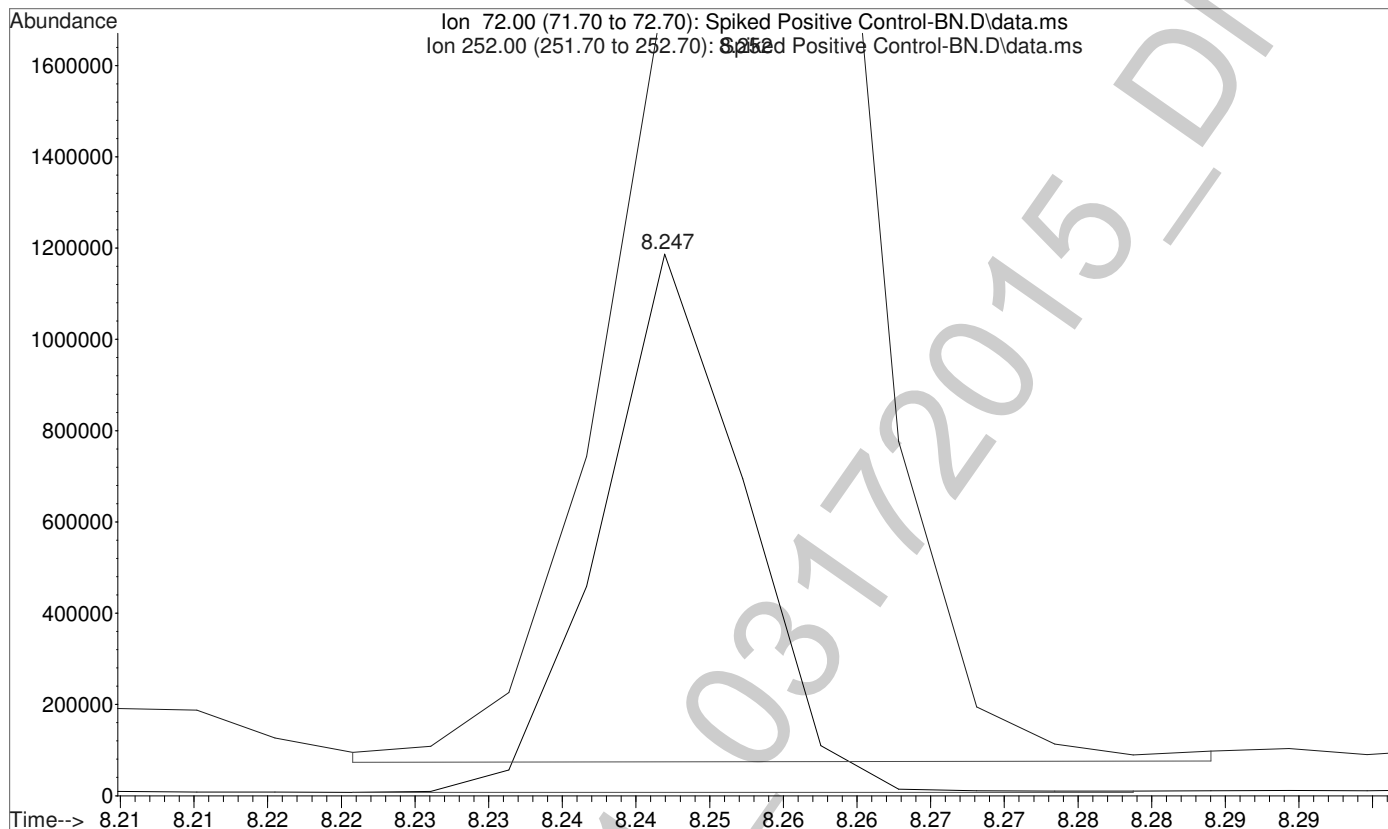



File :C:\gcms\1\data\Blood\031715BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 17 Mar 2015 18:25 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

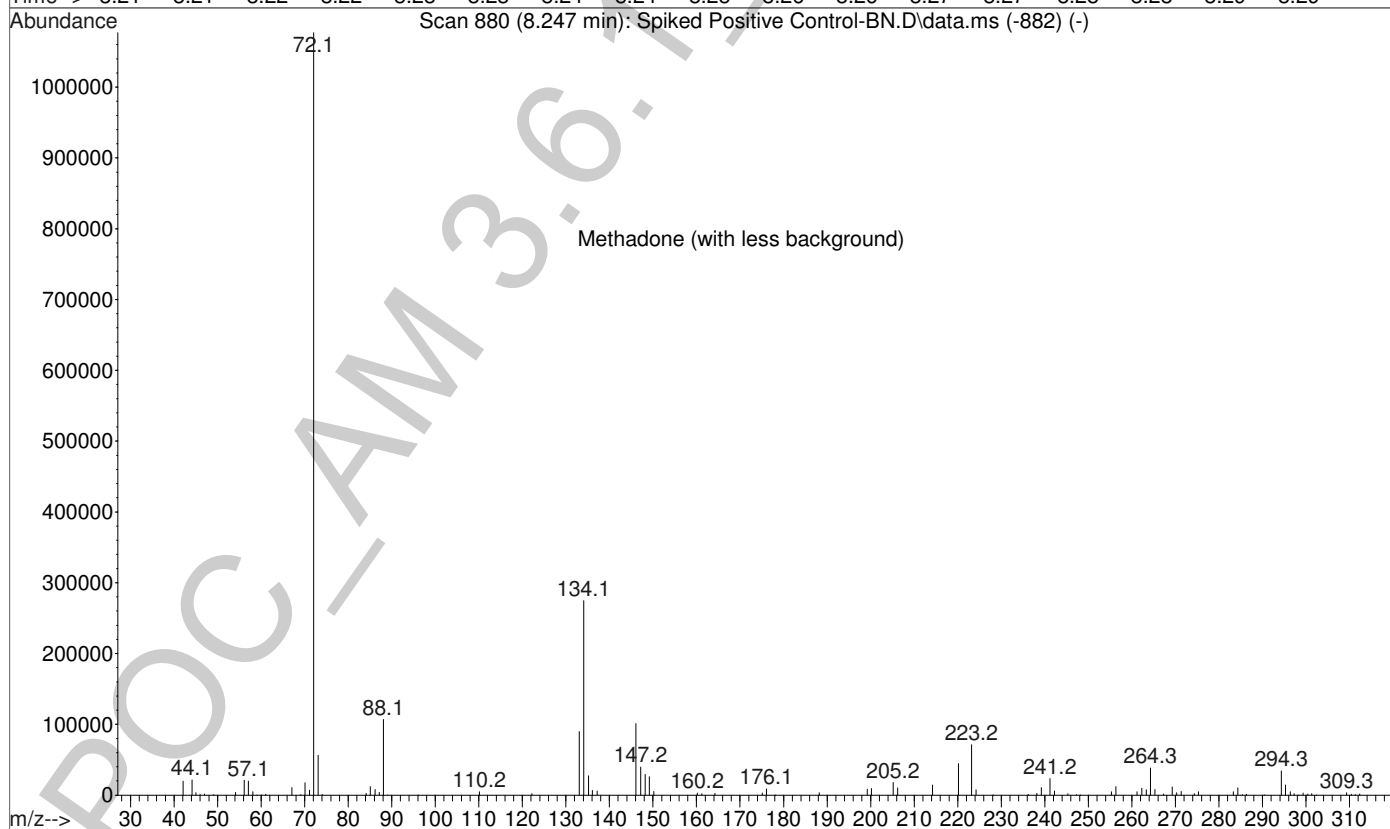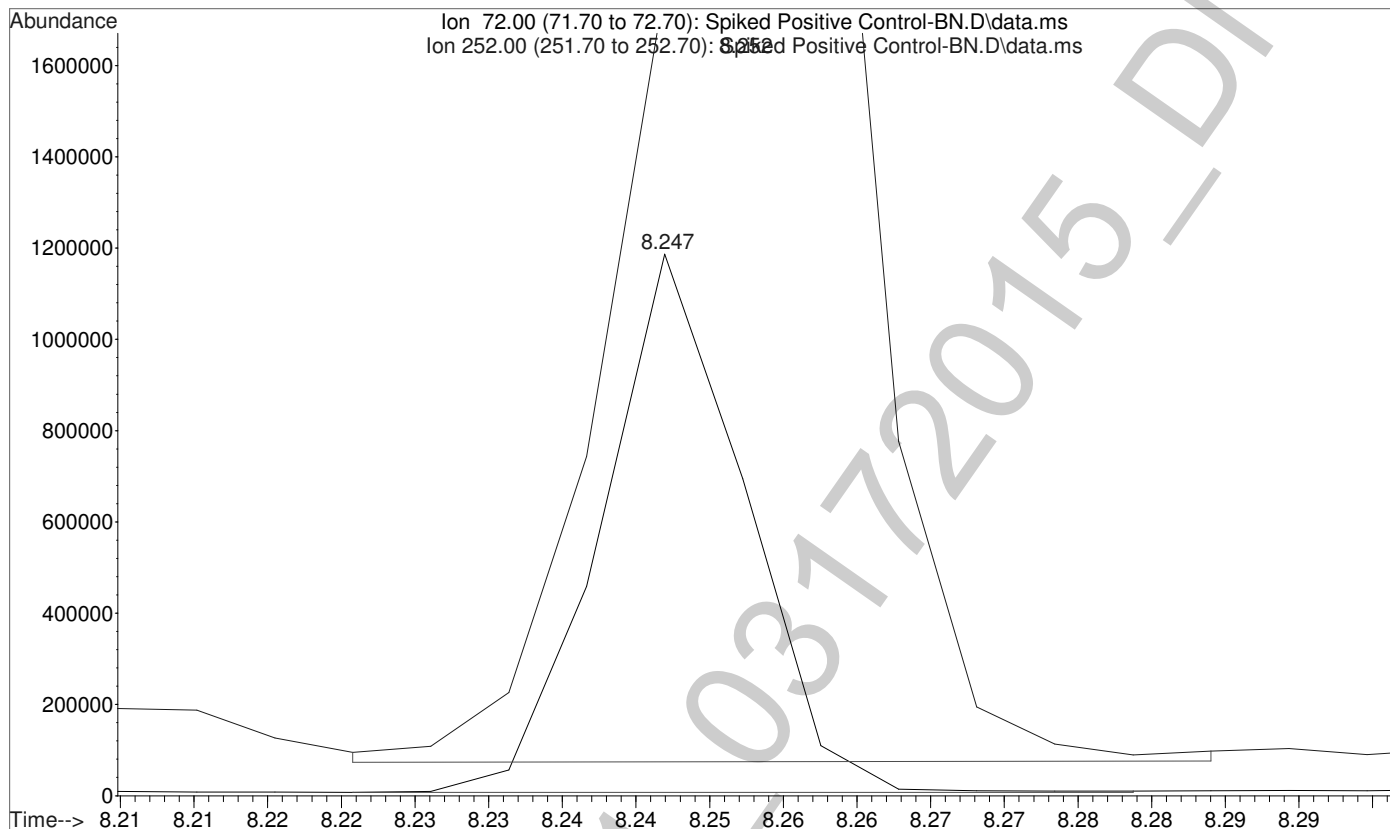



File :C:\gcms\1\data\Blood\031715BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 17 Mar 2015 18:25 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

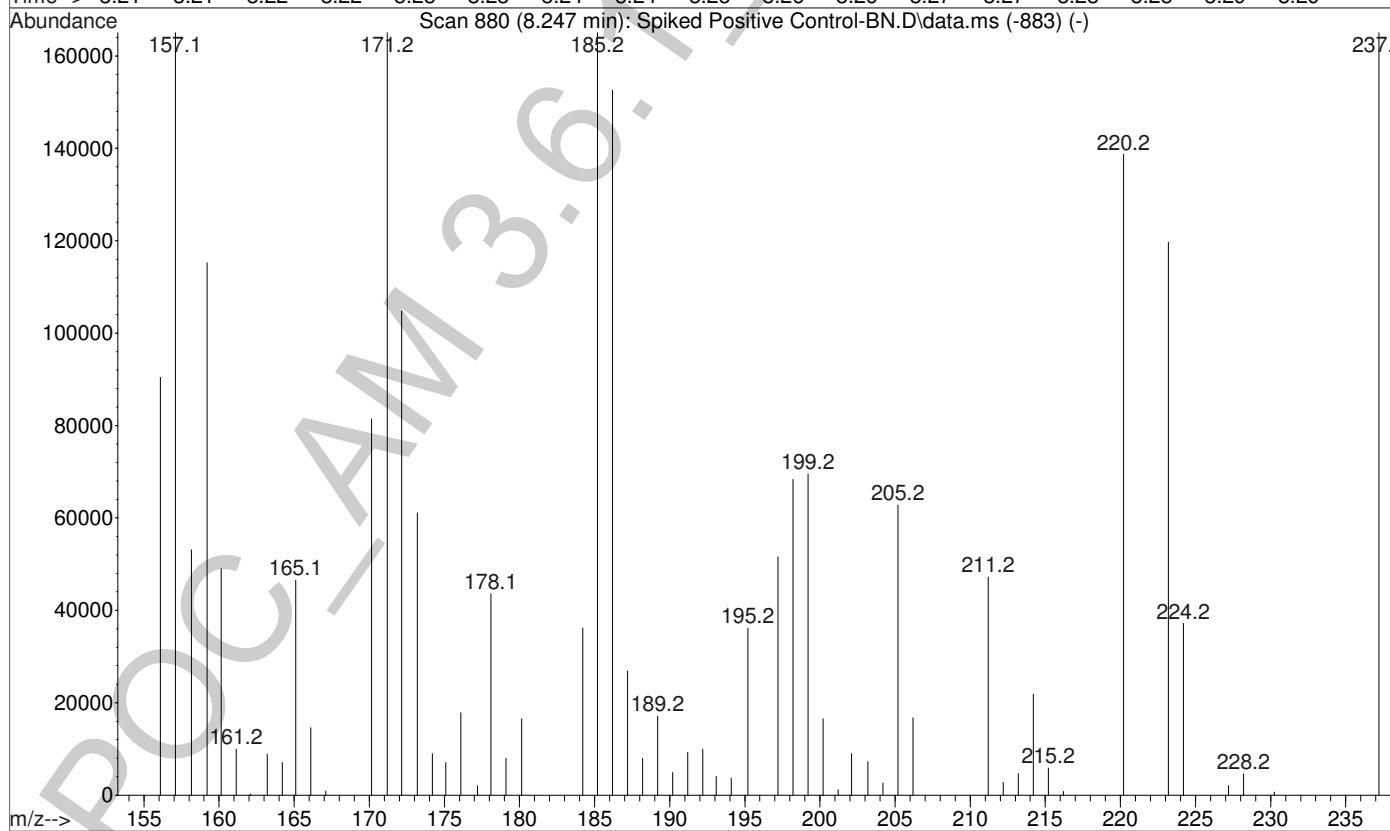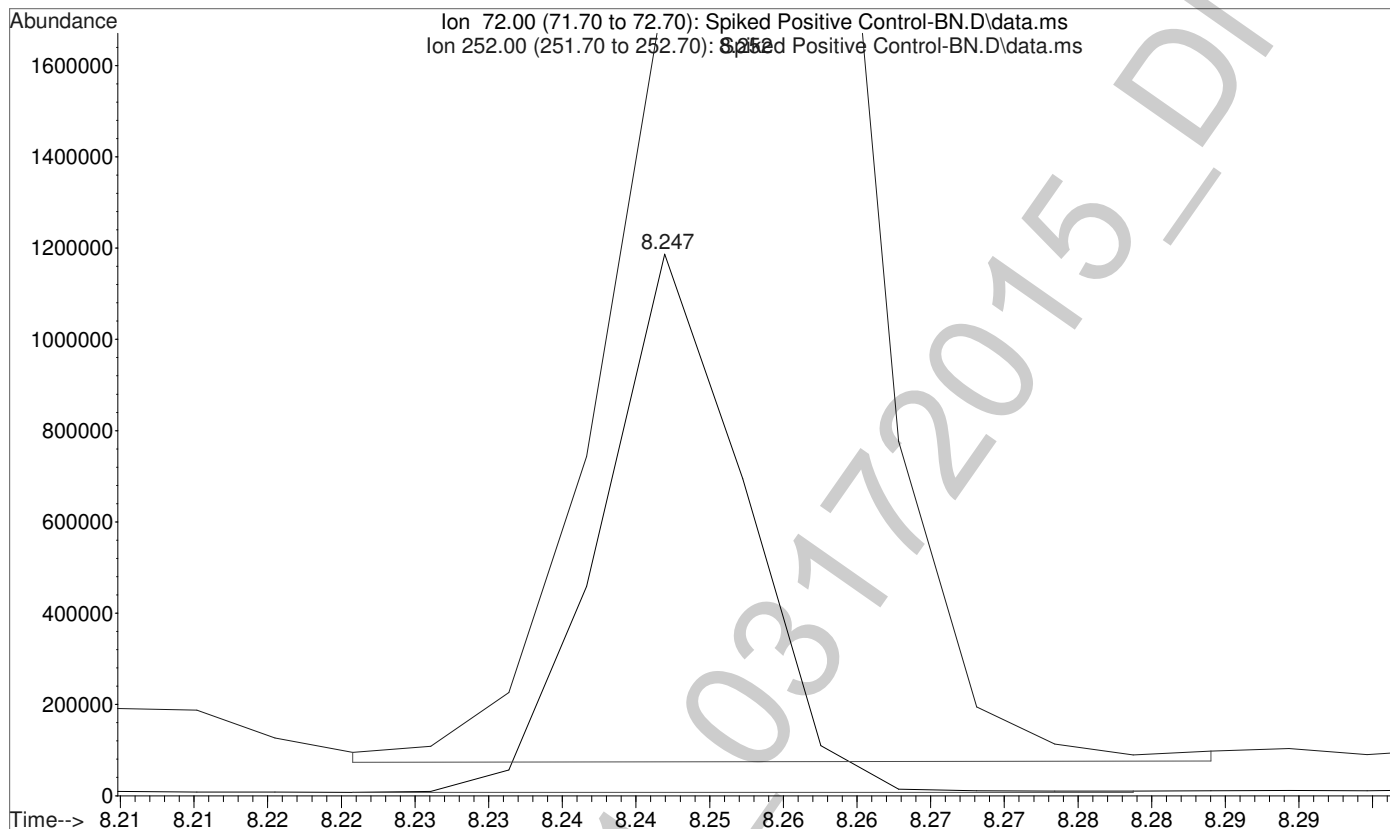



File :C:\gcms\1\data\Blood\031715BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 17 Mar 2015 18:25 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

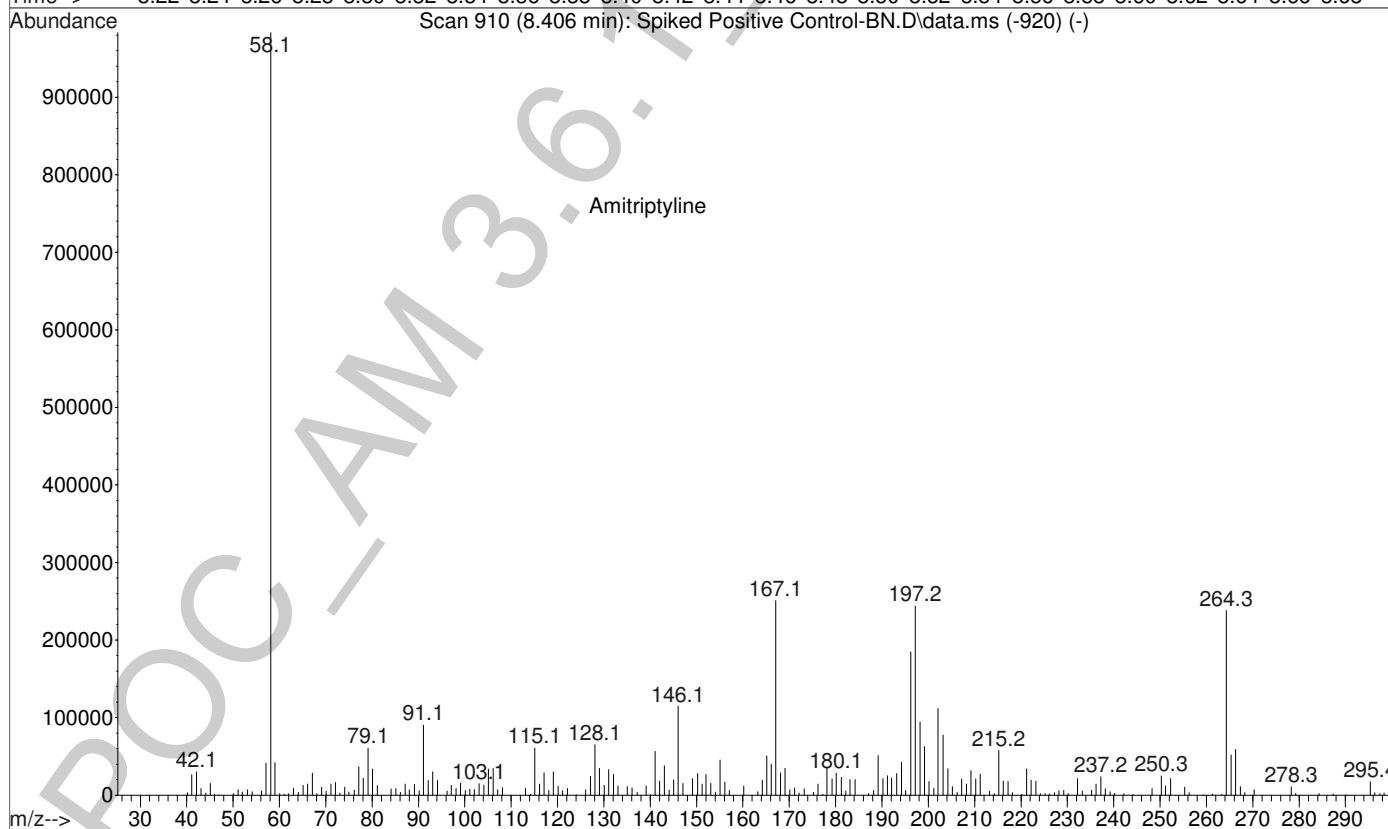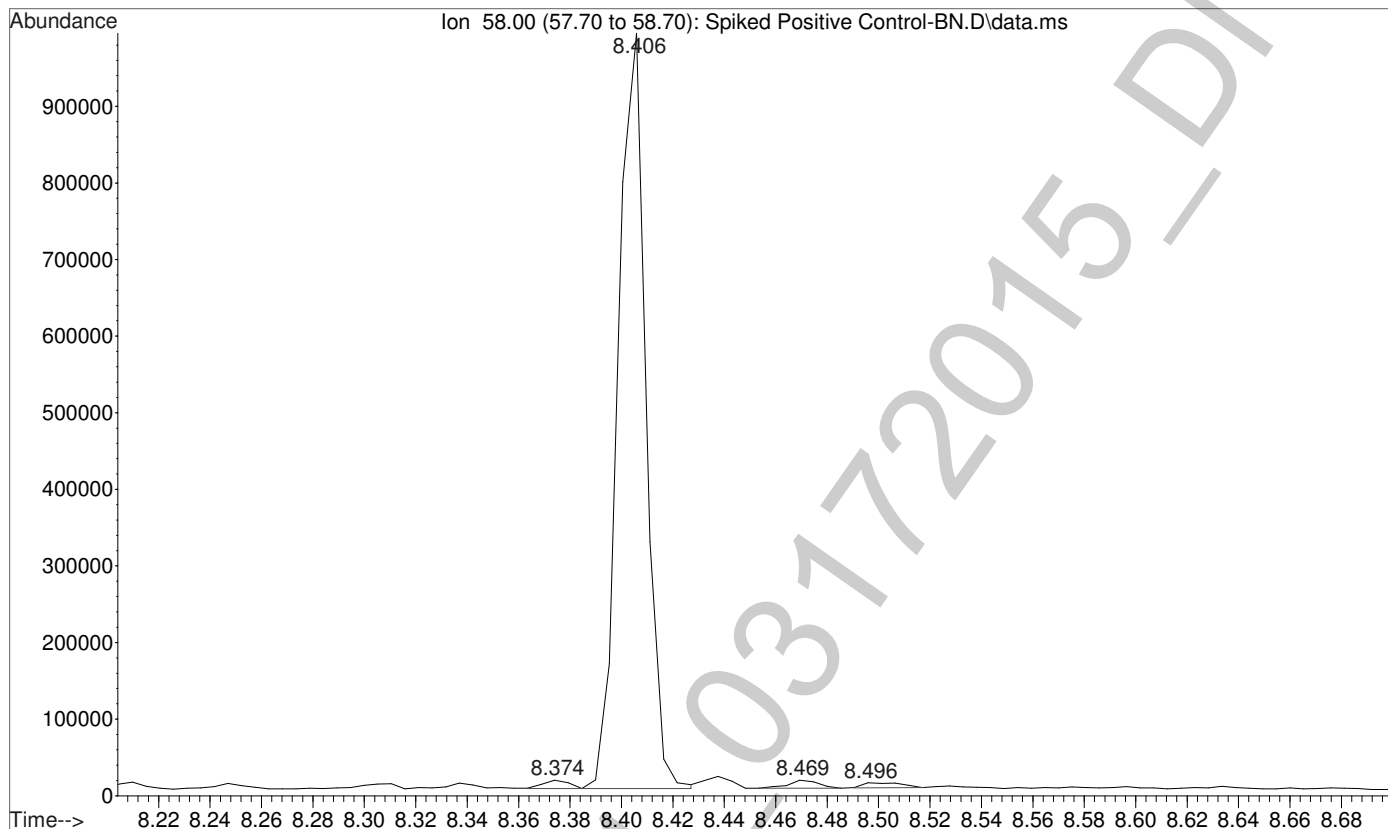



File :C:\gcms\1\data\Blood\031715BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 17 Mar 2015 18:25 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

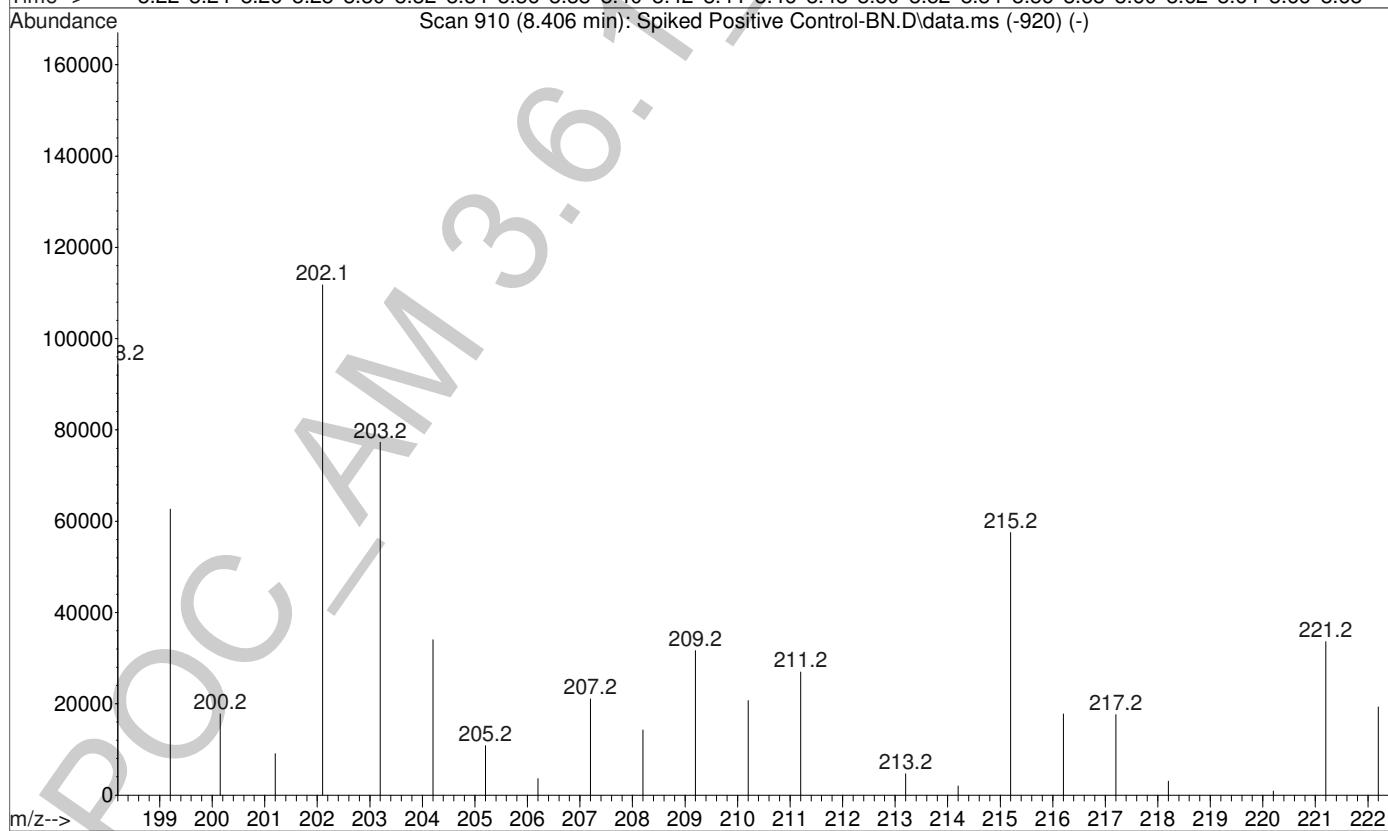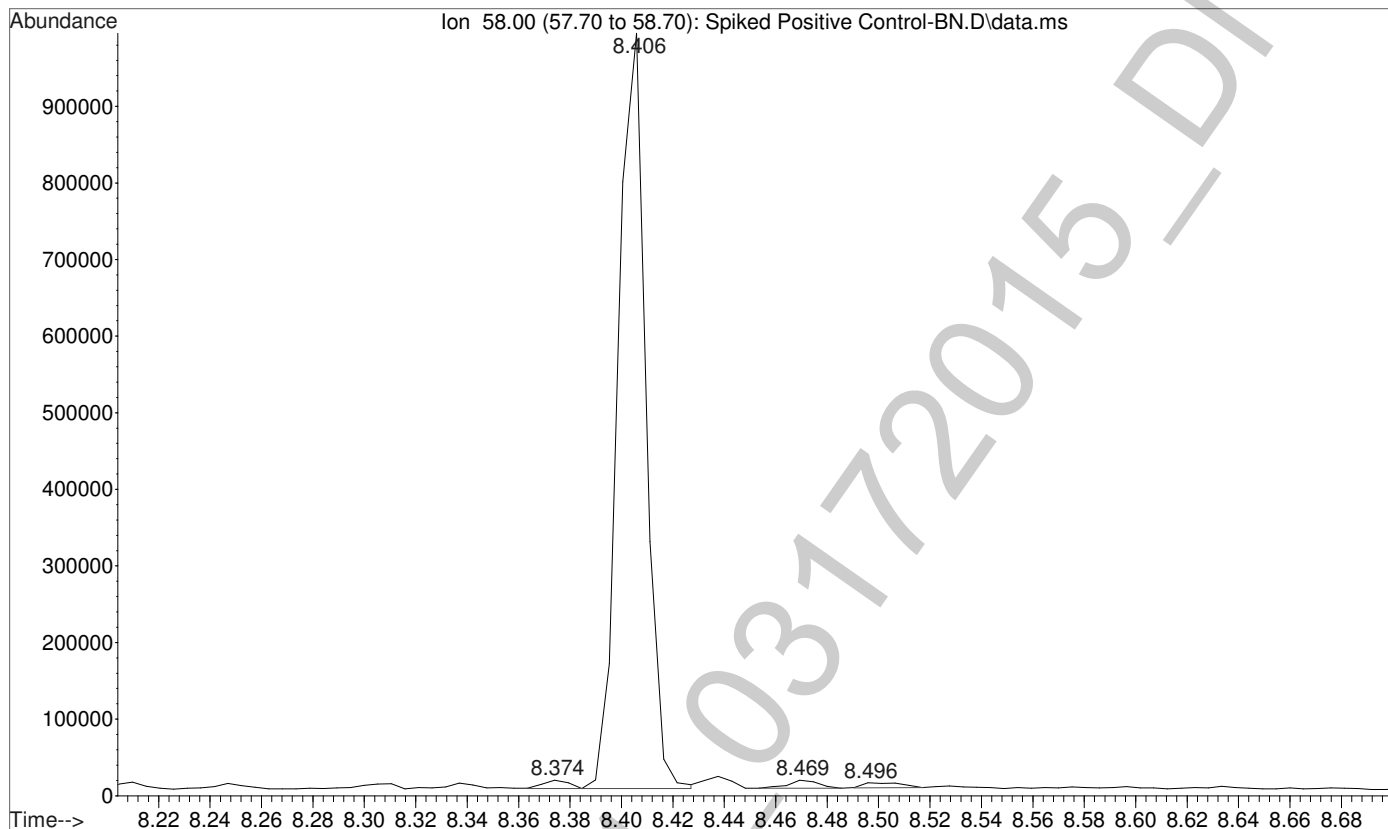



File :C:\gcms\1\data\Blood\031715BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 17 Mar 2015 18:25 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

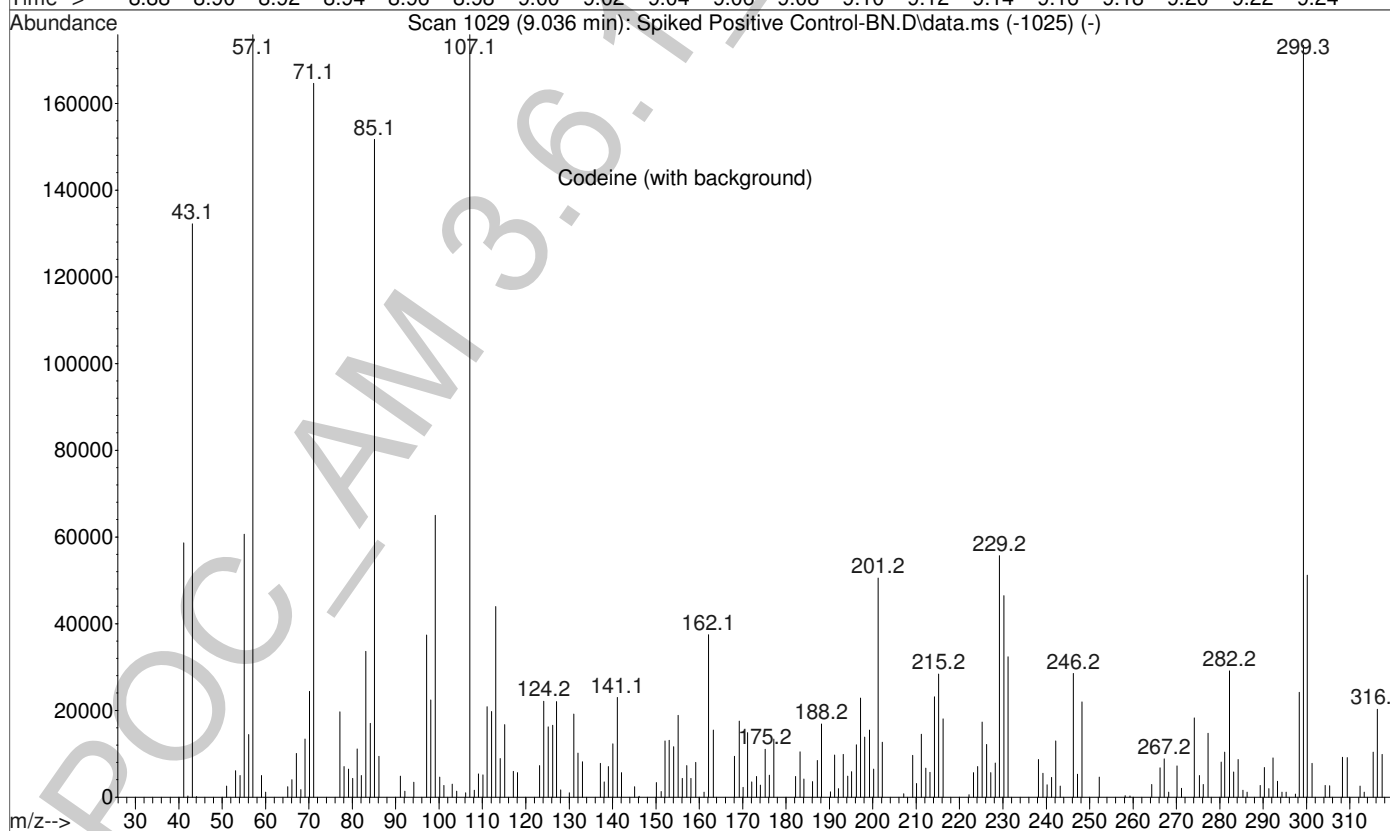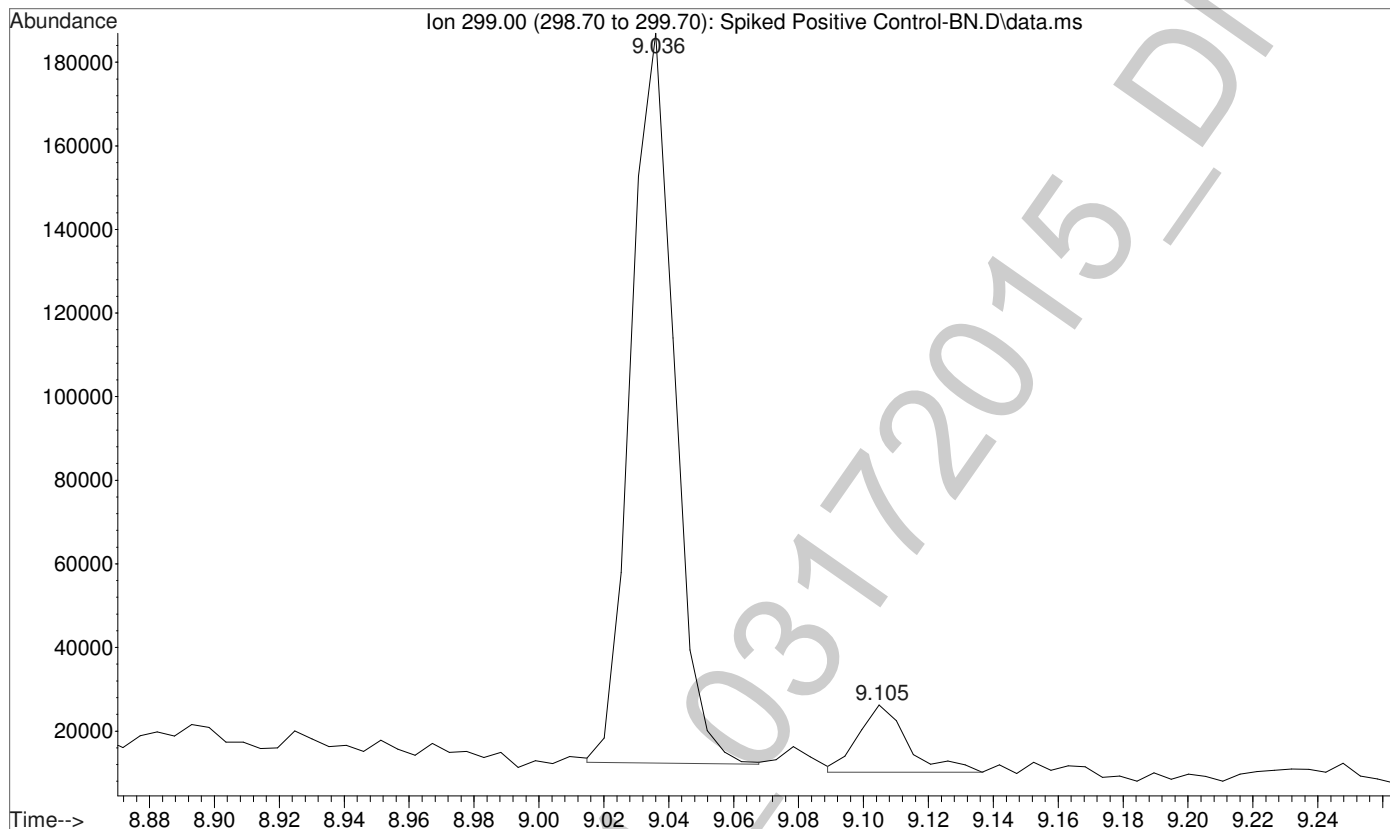

File :C:\gcms\1\data\Blood\031715BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 17 Mar 2015 18:25 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

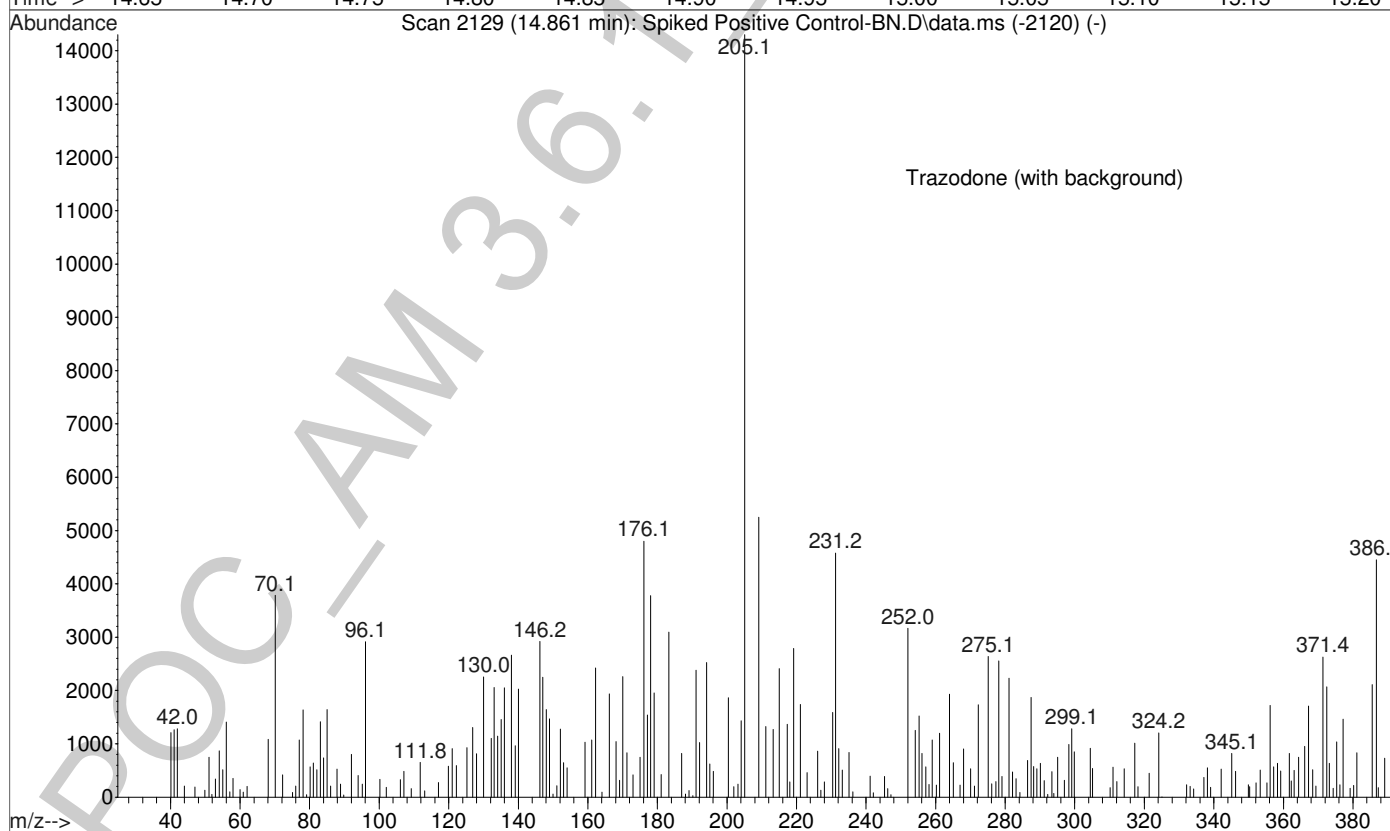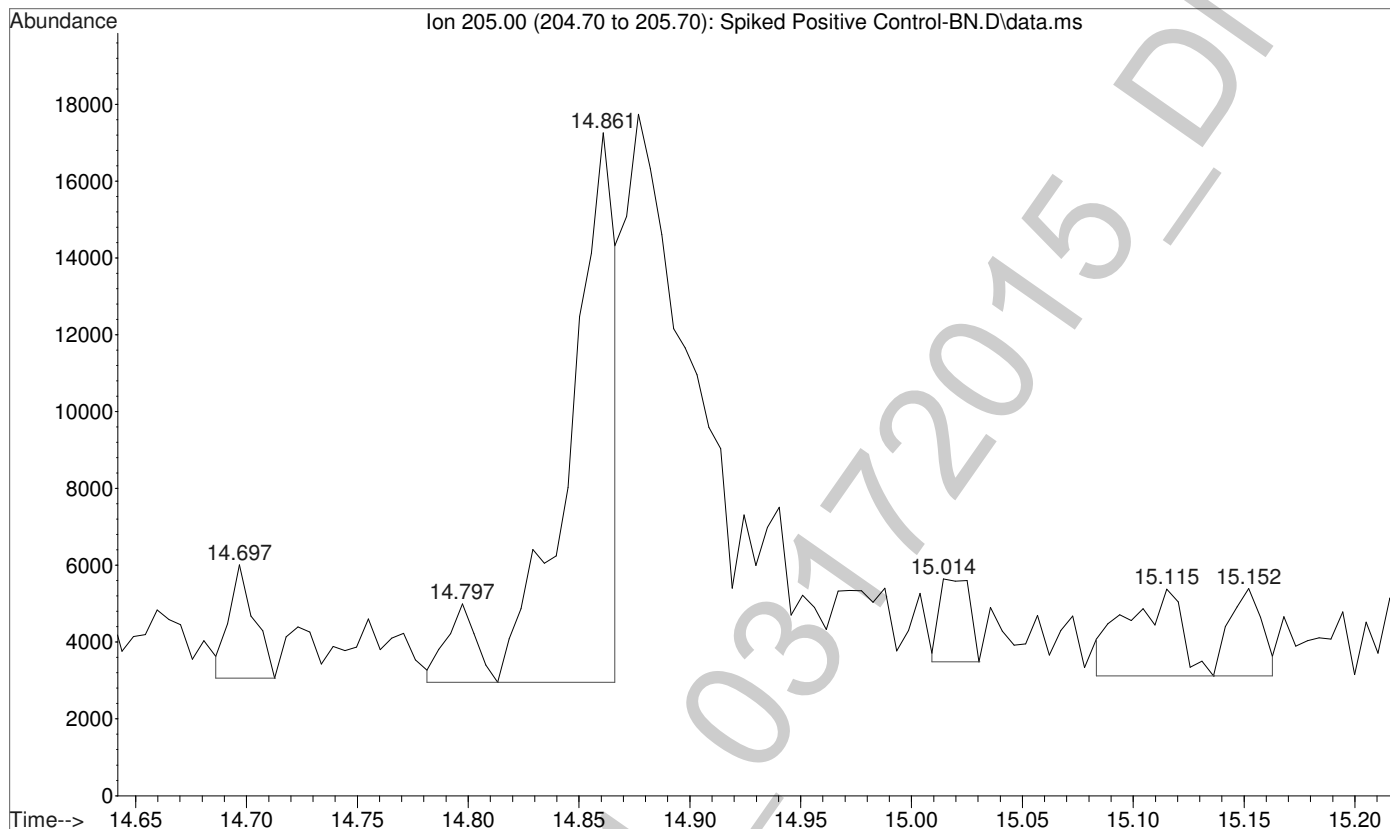

File :C:\gcms\1\data\Blood\031715BN\prbLK2.D
Operator : 5LAB-C01\ISPuser
Acquired : 17 Mar 2015 18:48 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Solvent Blank
Misc Info : Chloroform
Vial Number: 99

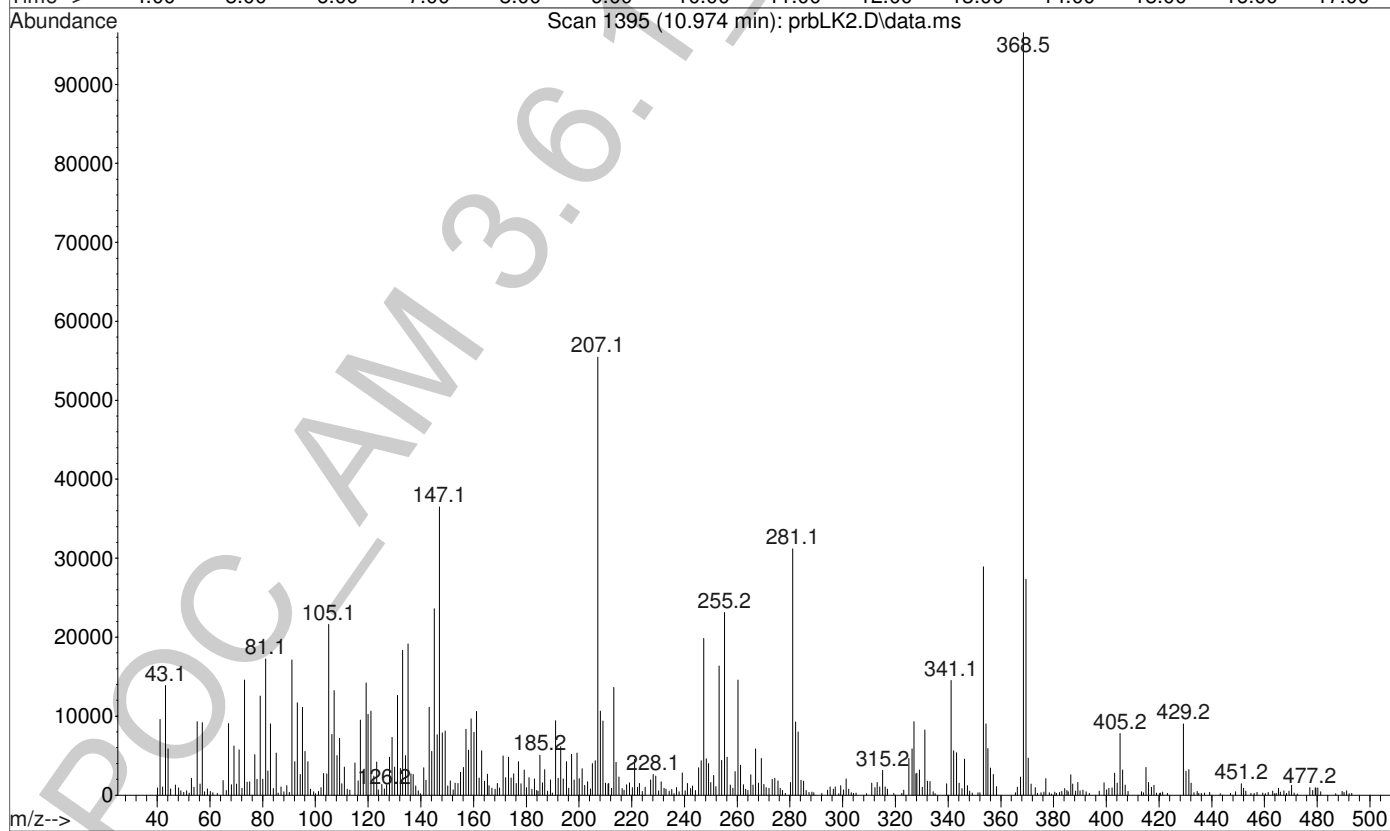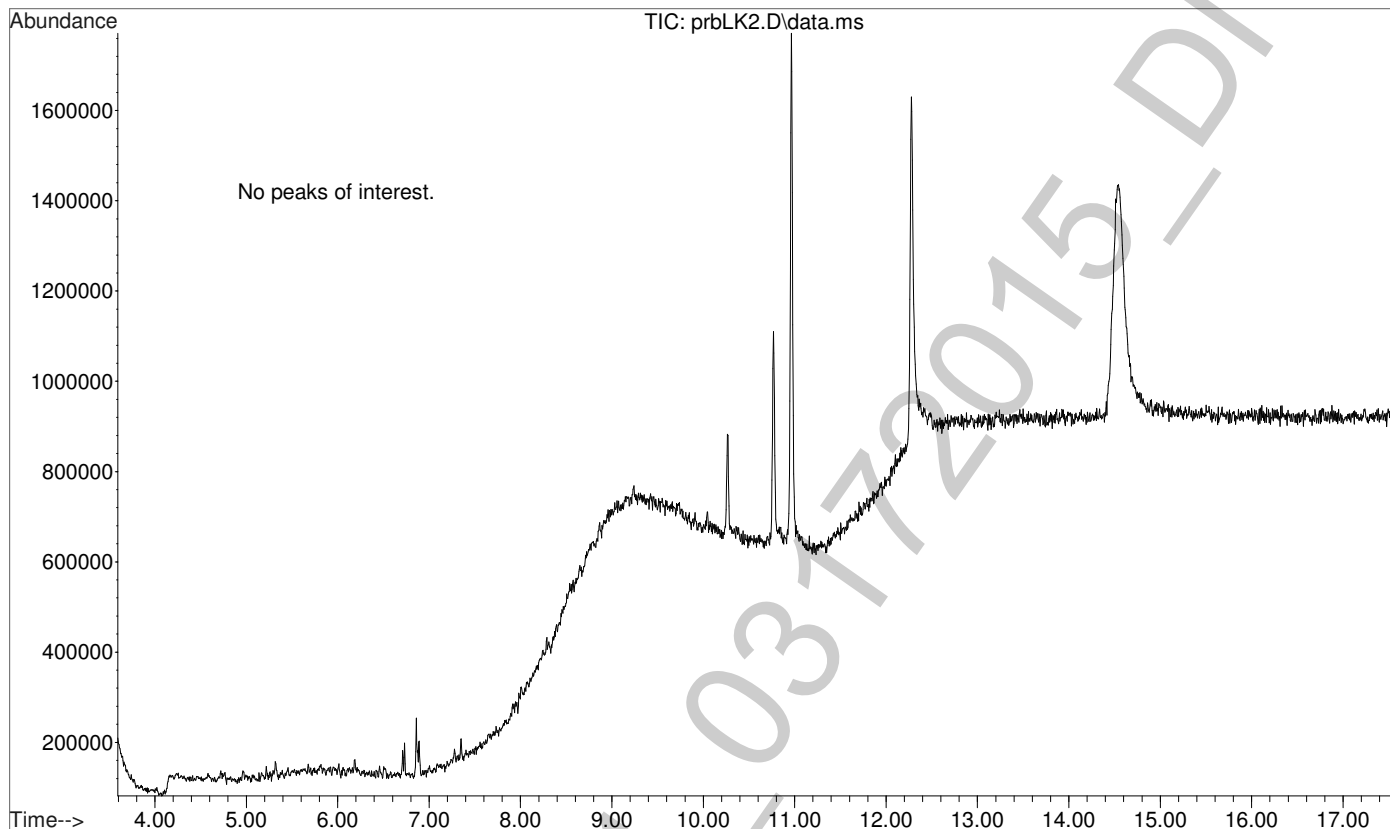


Analytical Method 3.6.1 & 3.6.7 QA Check List

Run Start Date: 03/17/15

Analyst: DND

(Long GC/MS temperature program)



Positive Control Compound List

- Methamphetamine
- Nicotine
- Meperidine
- Caffeine
- Diphenhydramine
- Lidocaine
- PCP
- Methadone
- Amitriptyline
- Codeine
- Trazodone



Internal Standards

- Benzphetamine
- Papaverine


Optional back extraction **not** performed.
Samples reconstituted in methanol.

POC_AM_3.6.1_03172015_DND



File :C:\gcms\1\data\Blood\031715BN\Reinjection Longer GC Method\P
... rerun Solvent Blankr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 17 Mar 2015 19:10 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Pre-run Solvent Blank
Misc Info : Chloroform

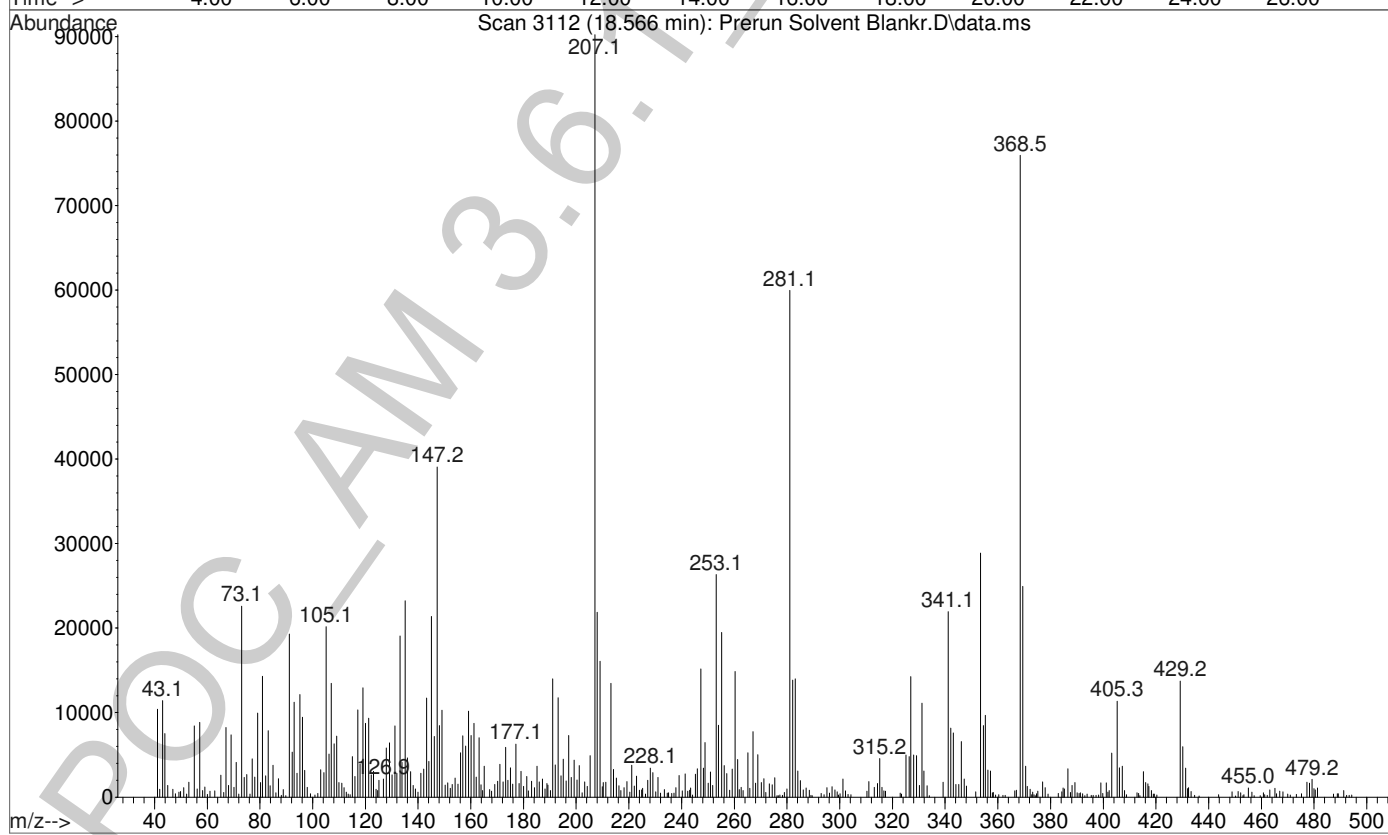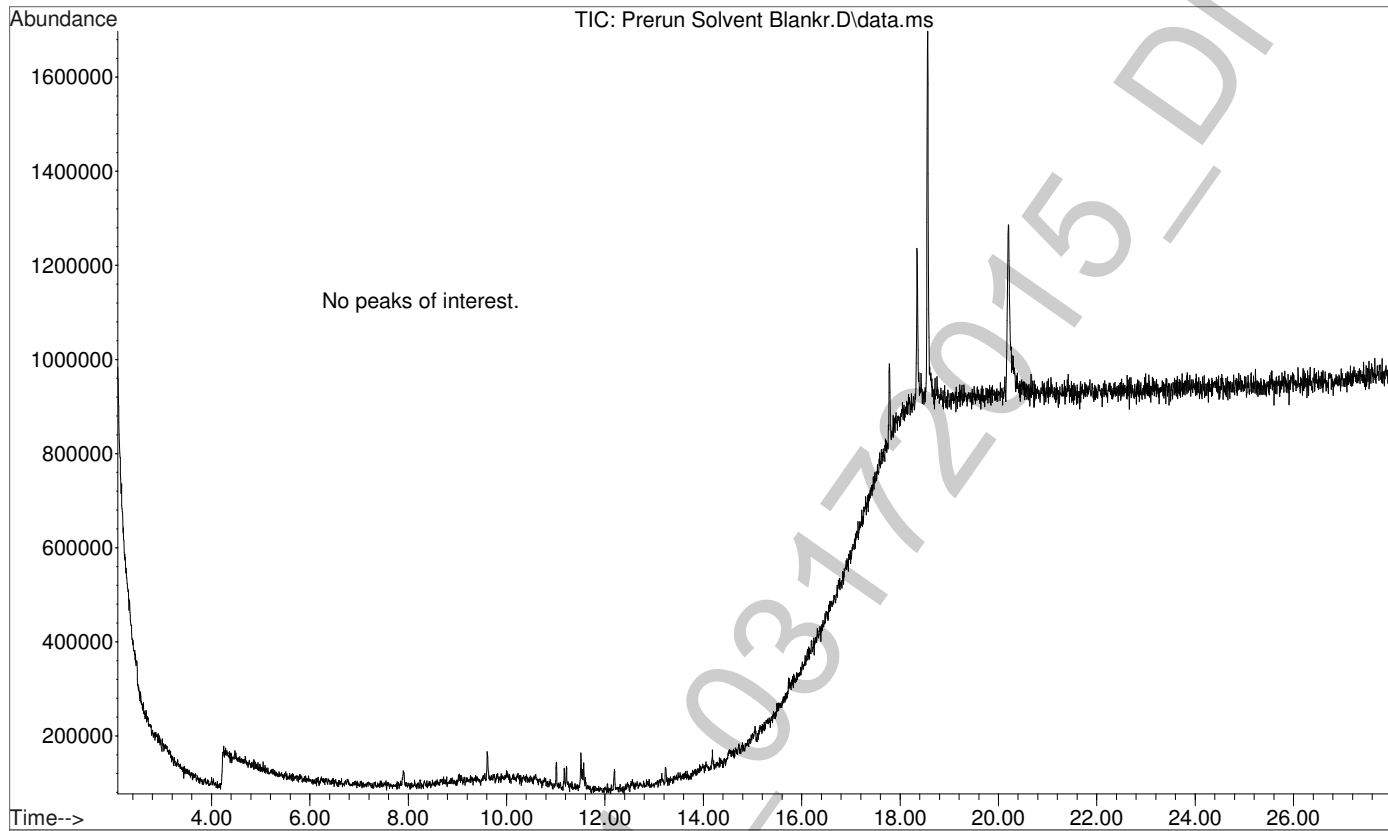



File :C:\gcms\1\data\Blood\031715BN\Reinjection Longer GC Method\N
... egative Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 17 Mar 2015 19:44 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Negative Control - Utak Lot B0130
Misc Info : Analytical Method 3.6.1

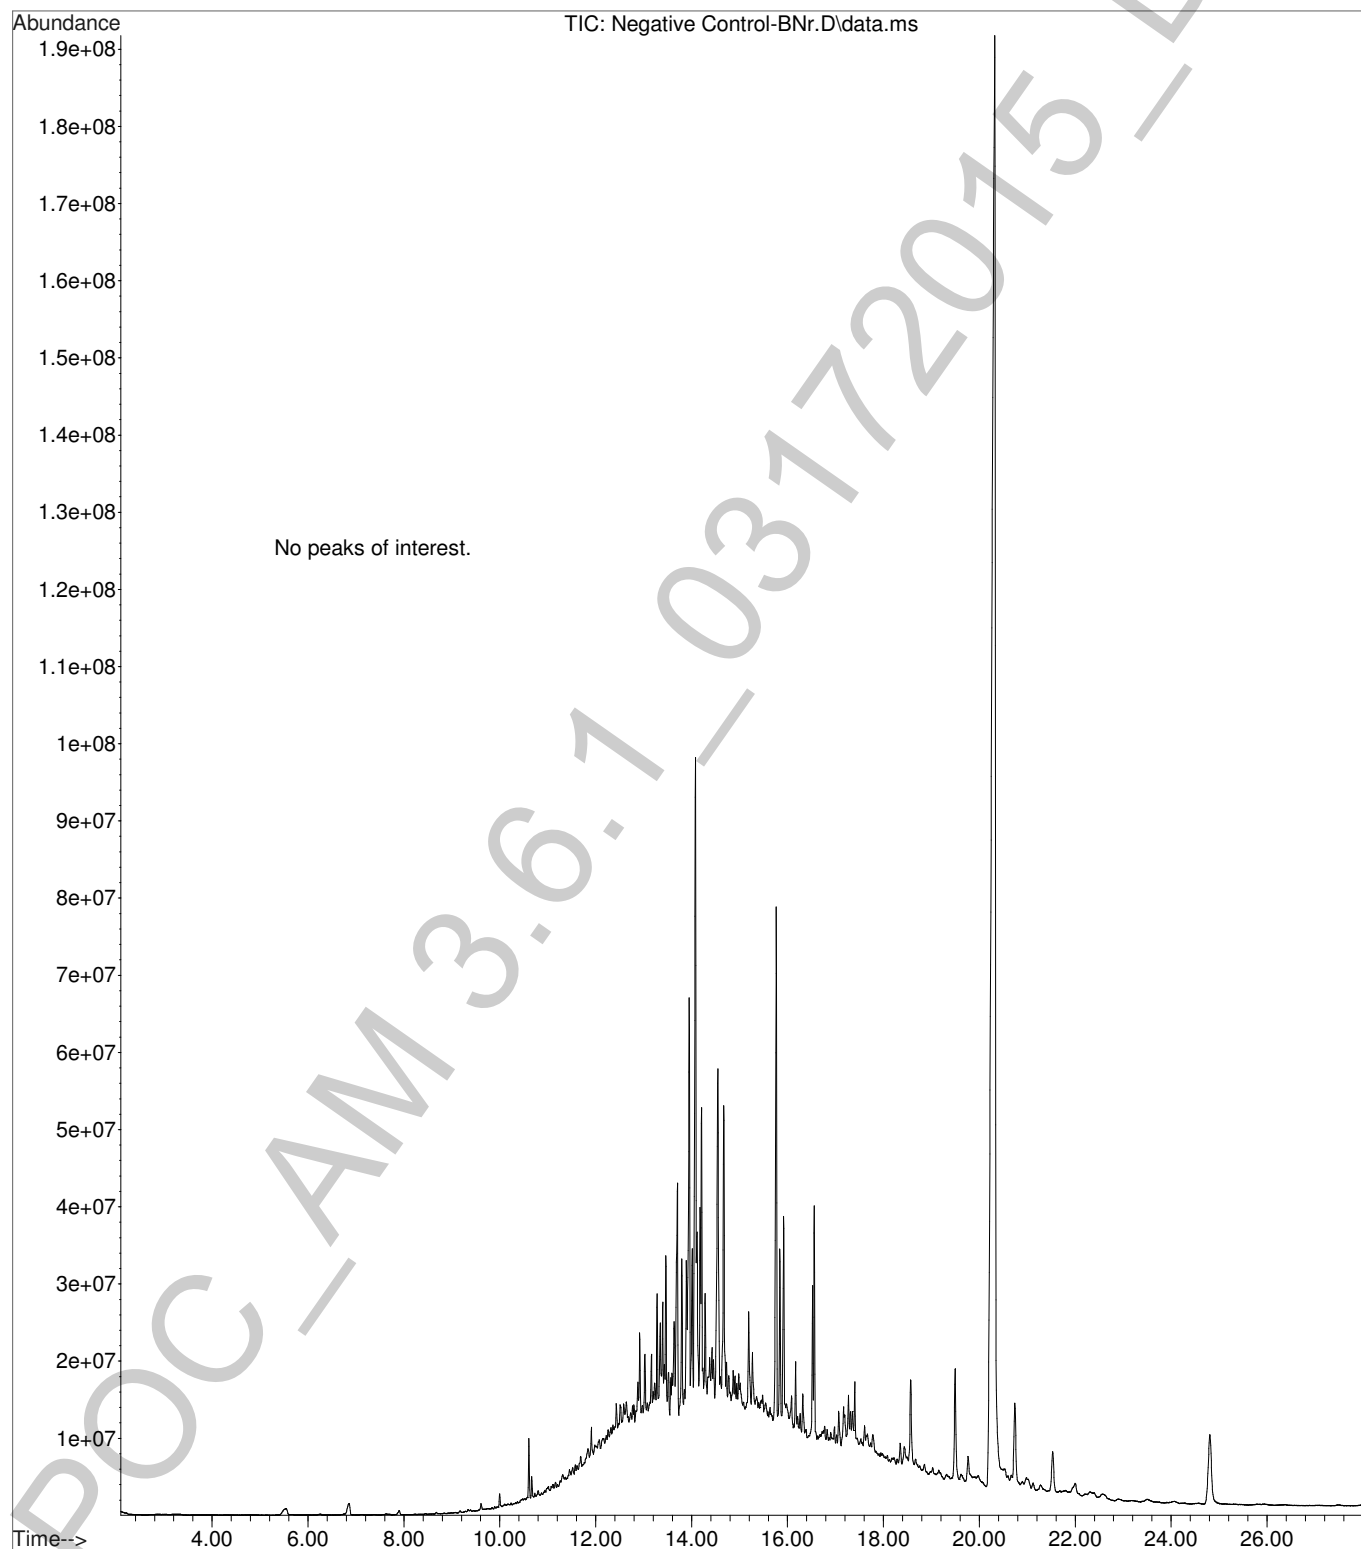


File :C:\gcms\1\data\Blood\031715BN\Reinjection Longer GC Method\N
... egative Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 17 Mar 2015 19:44 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Negative Control - Utak Lot B0130
Misc Info : Analytical Method 3.6.1

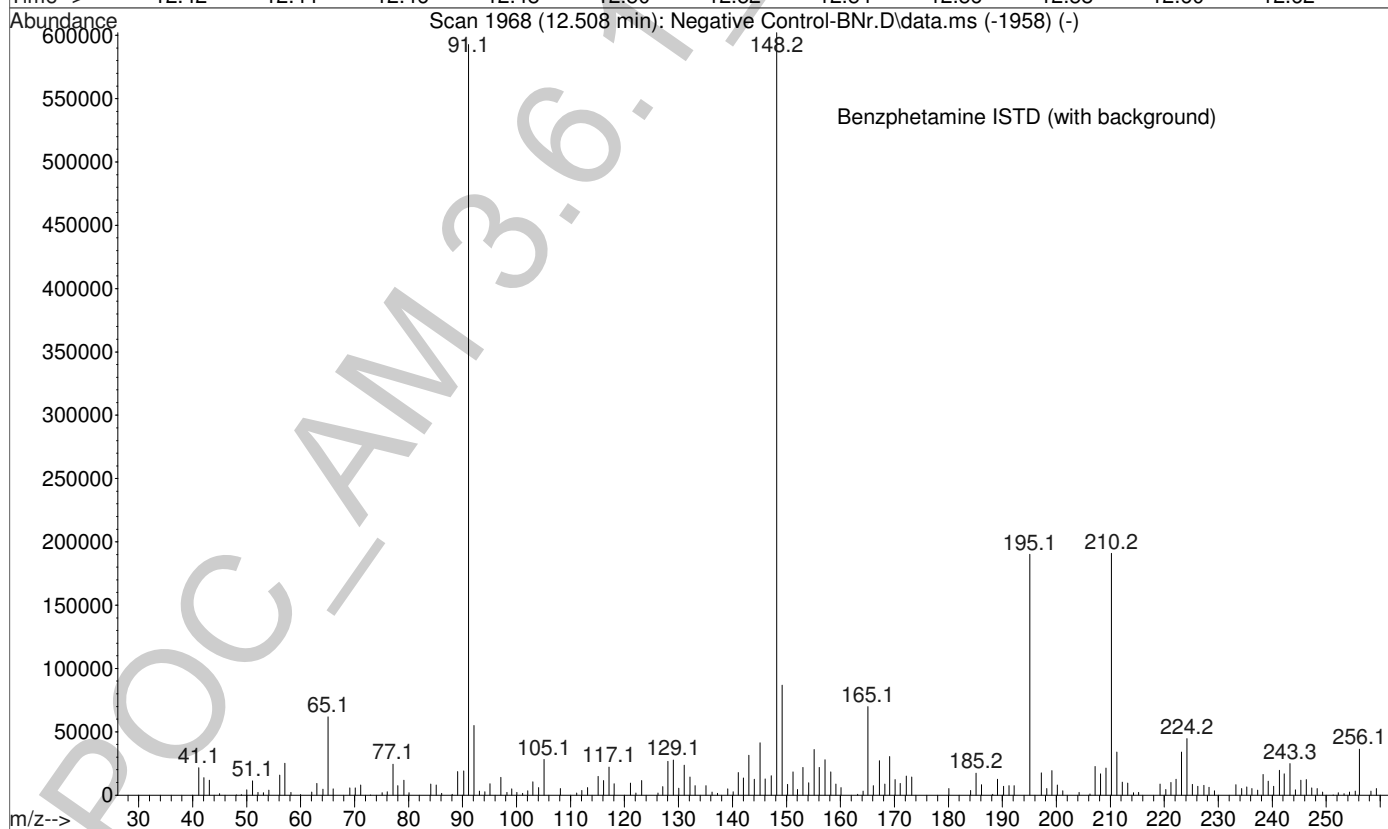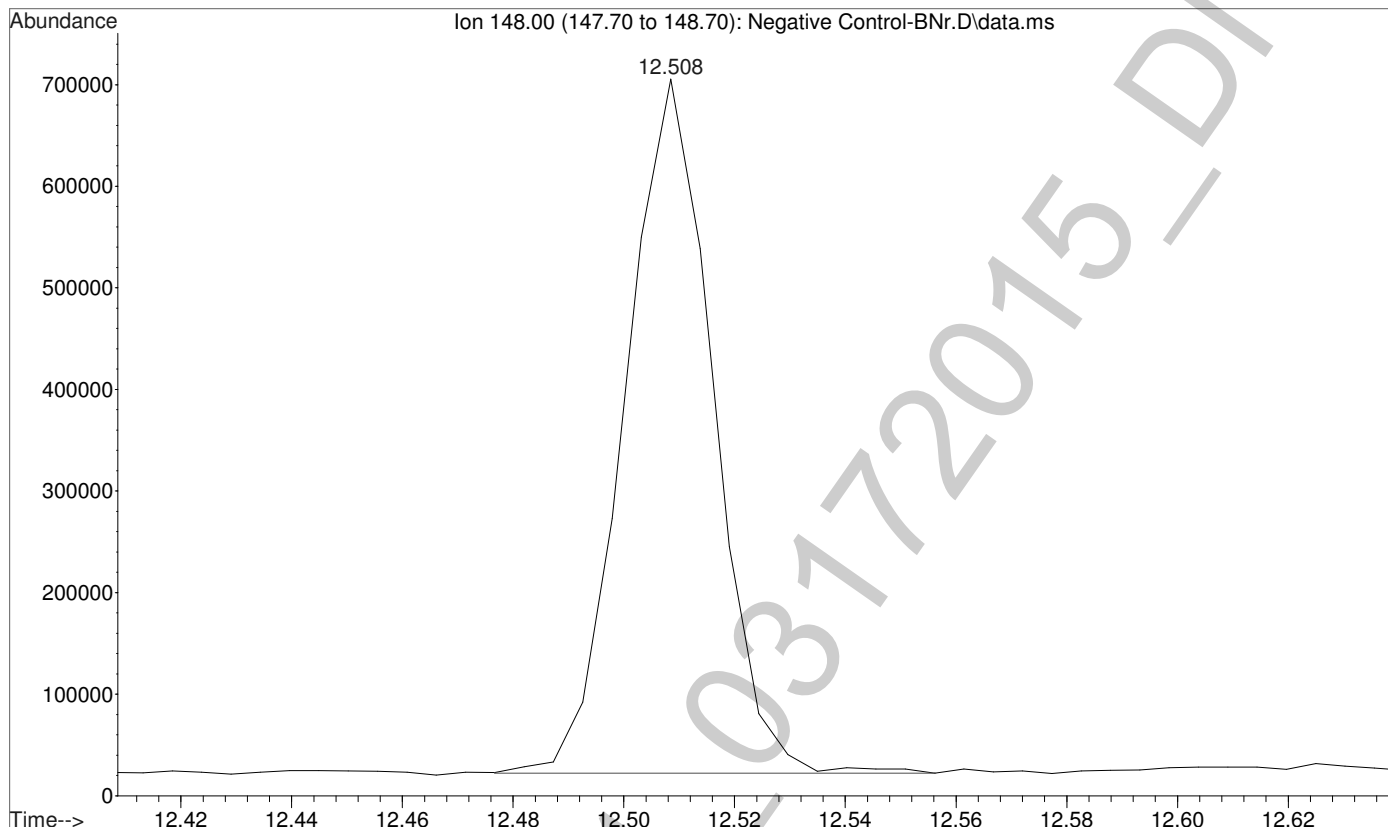



File :C:\gcms\1\data\Blood\031715BN\Reinjection Longer GC Method\N
... egative Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 17 Mar 2015 19:44 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Negative Control - Utak Lot B0130
Misc Info : Analytical Method 3.6.1

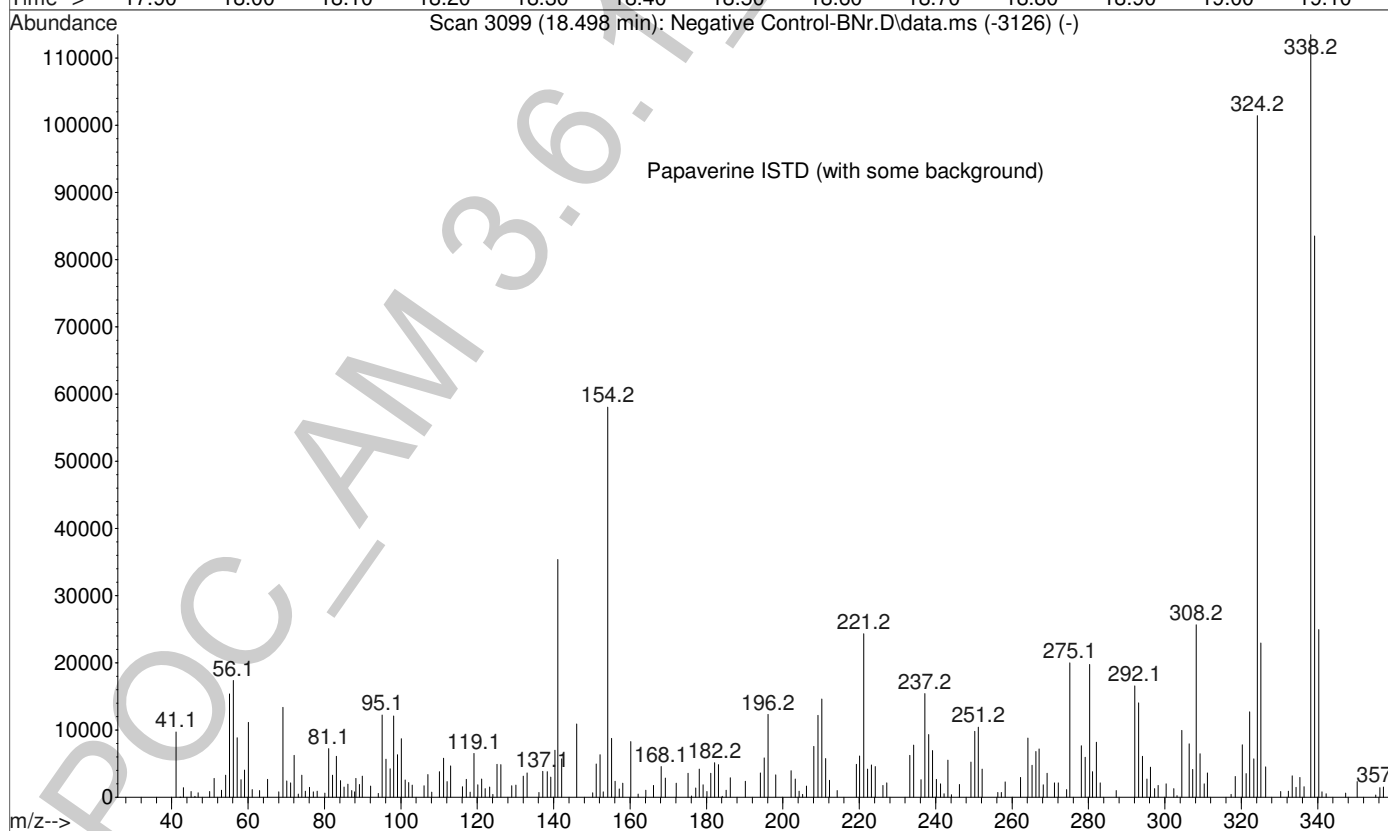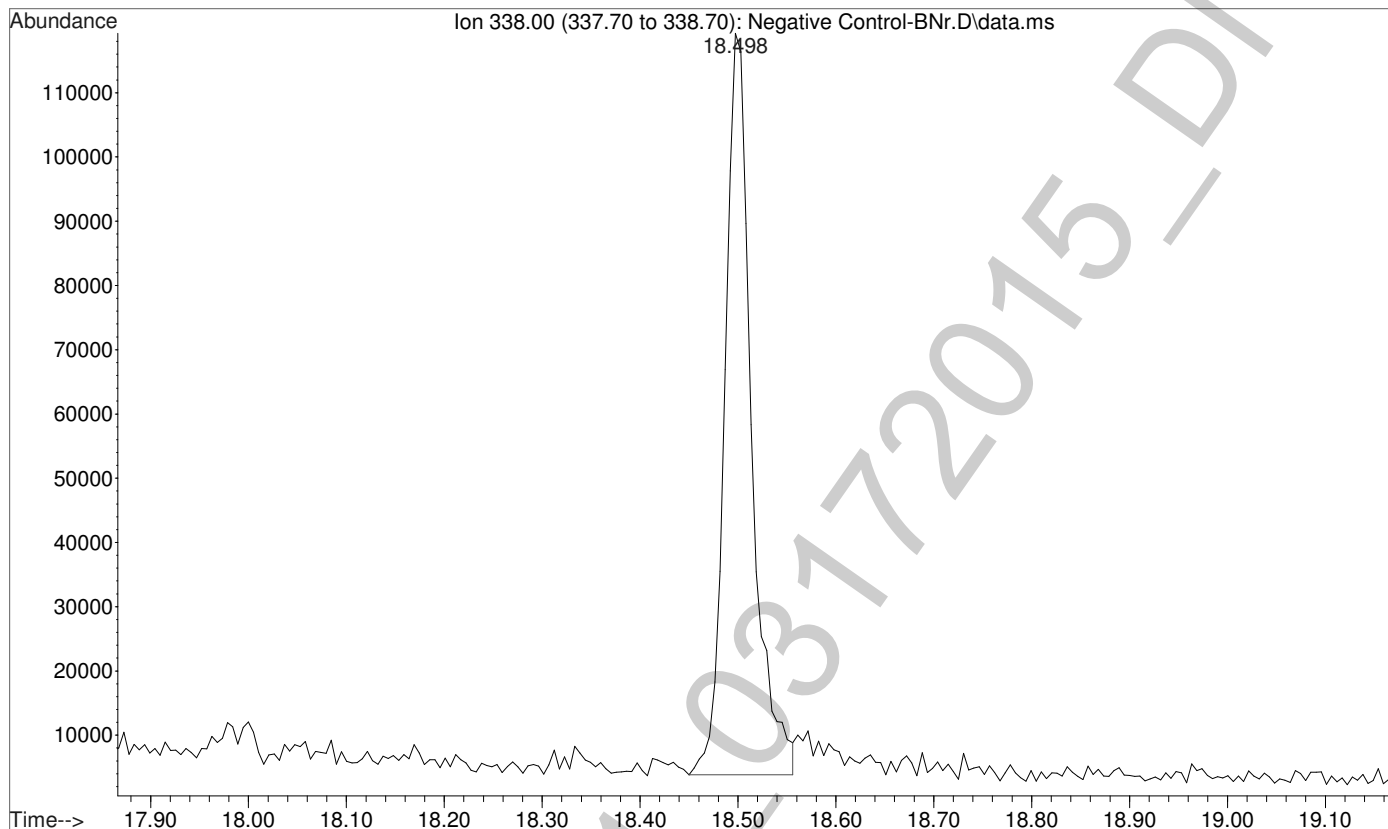



File :C:\gcms\1\data\Blood\031715BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 17 Mar 2015 20:18 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

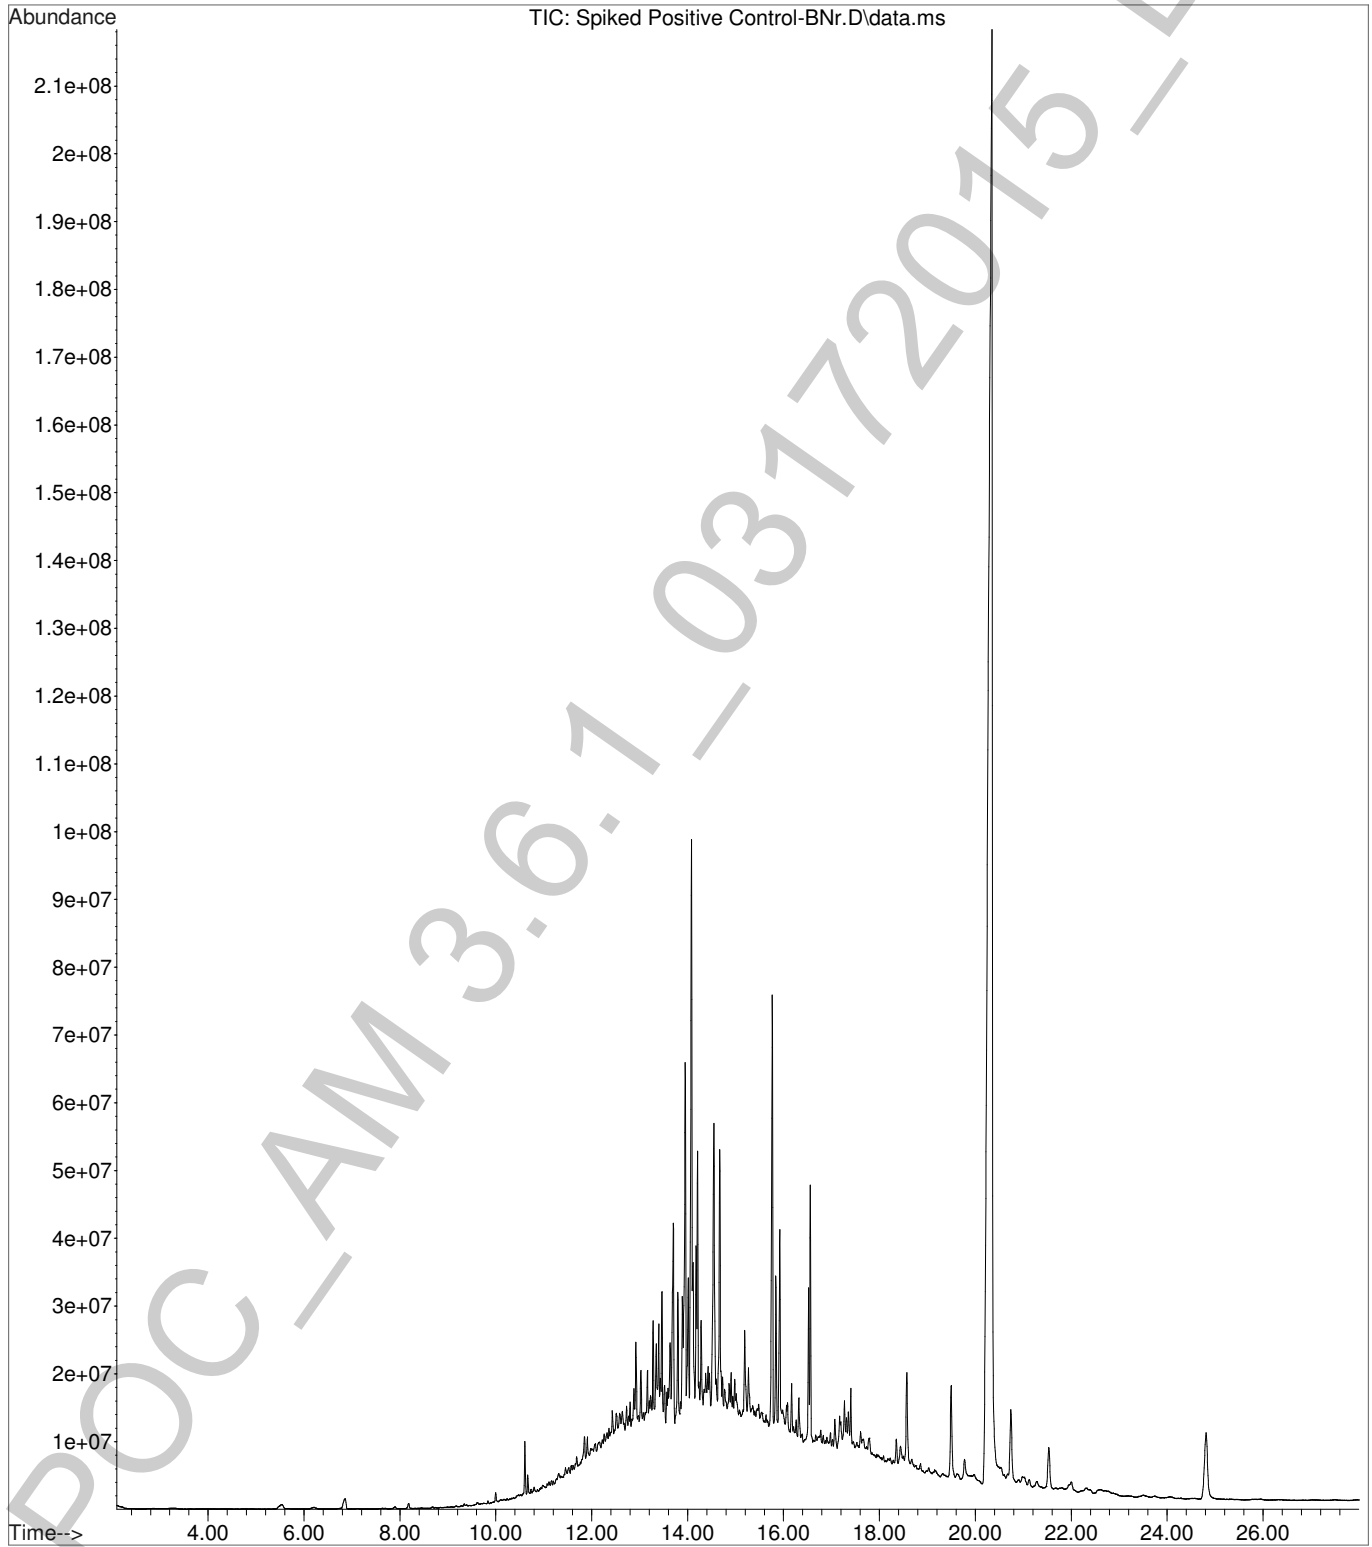



File :C:\gcms\1\data\Blood\031715BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 17 Mar 2015 20:18 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

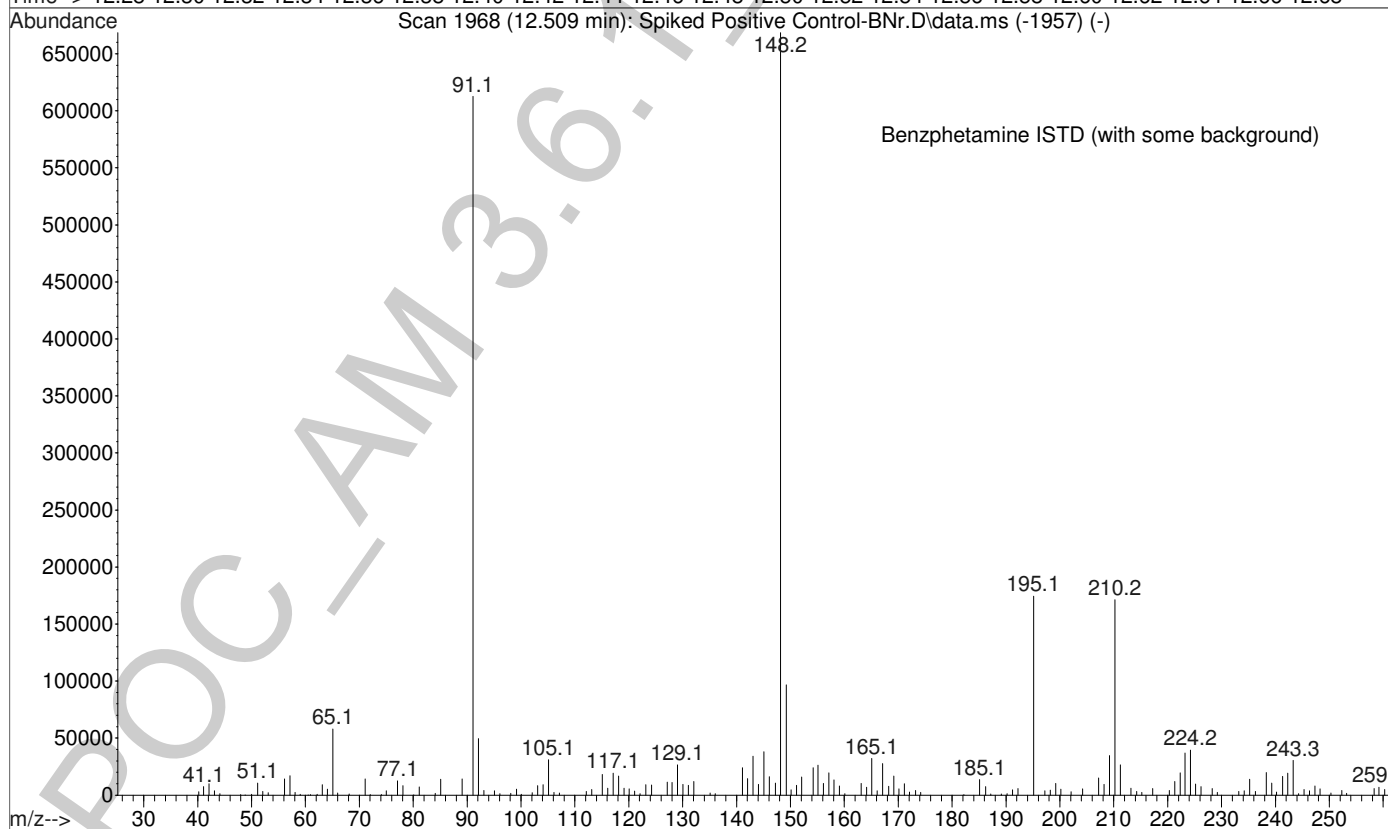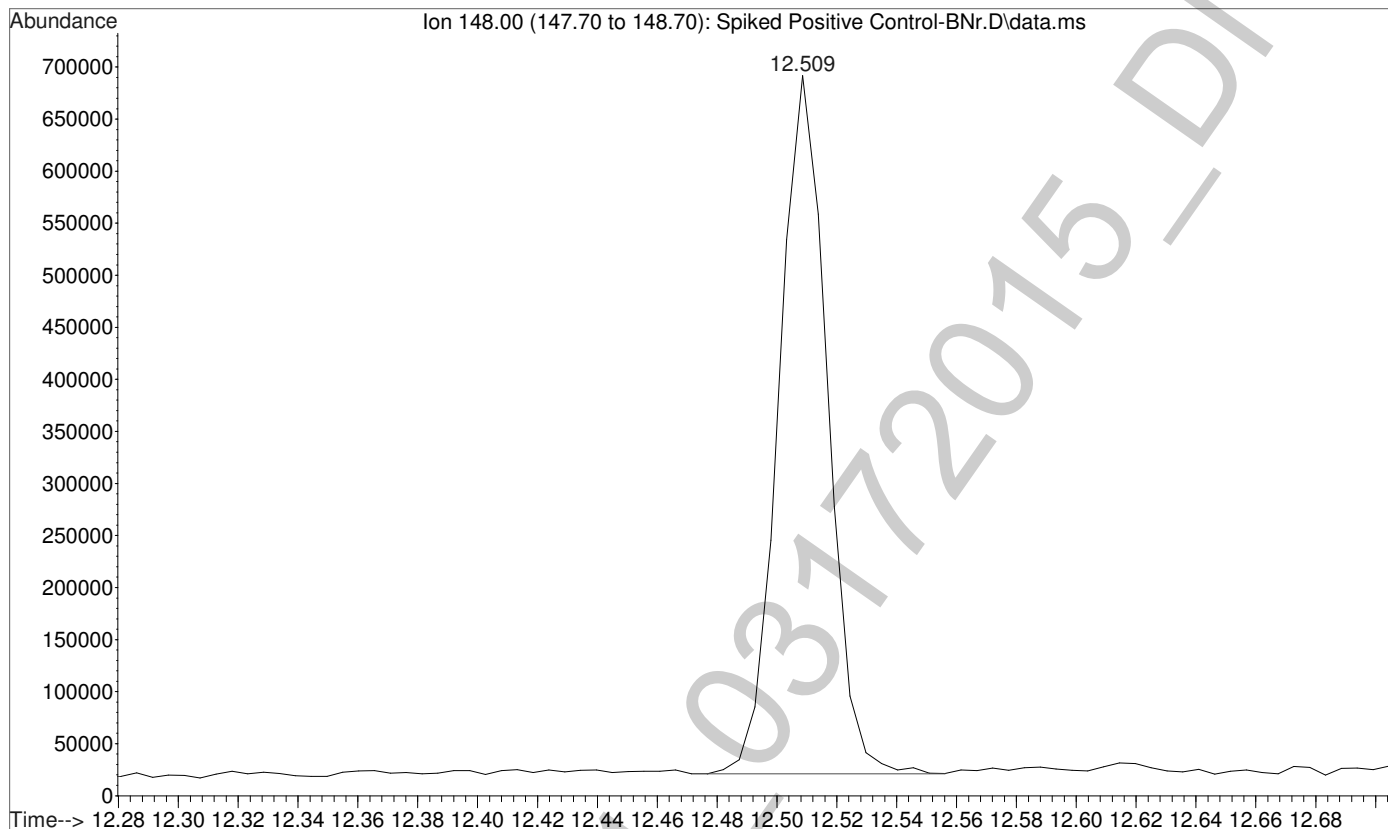



File :C:\gcms\1\data\Blood\031715BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 17 Mar 2015 20:18 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

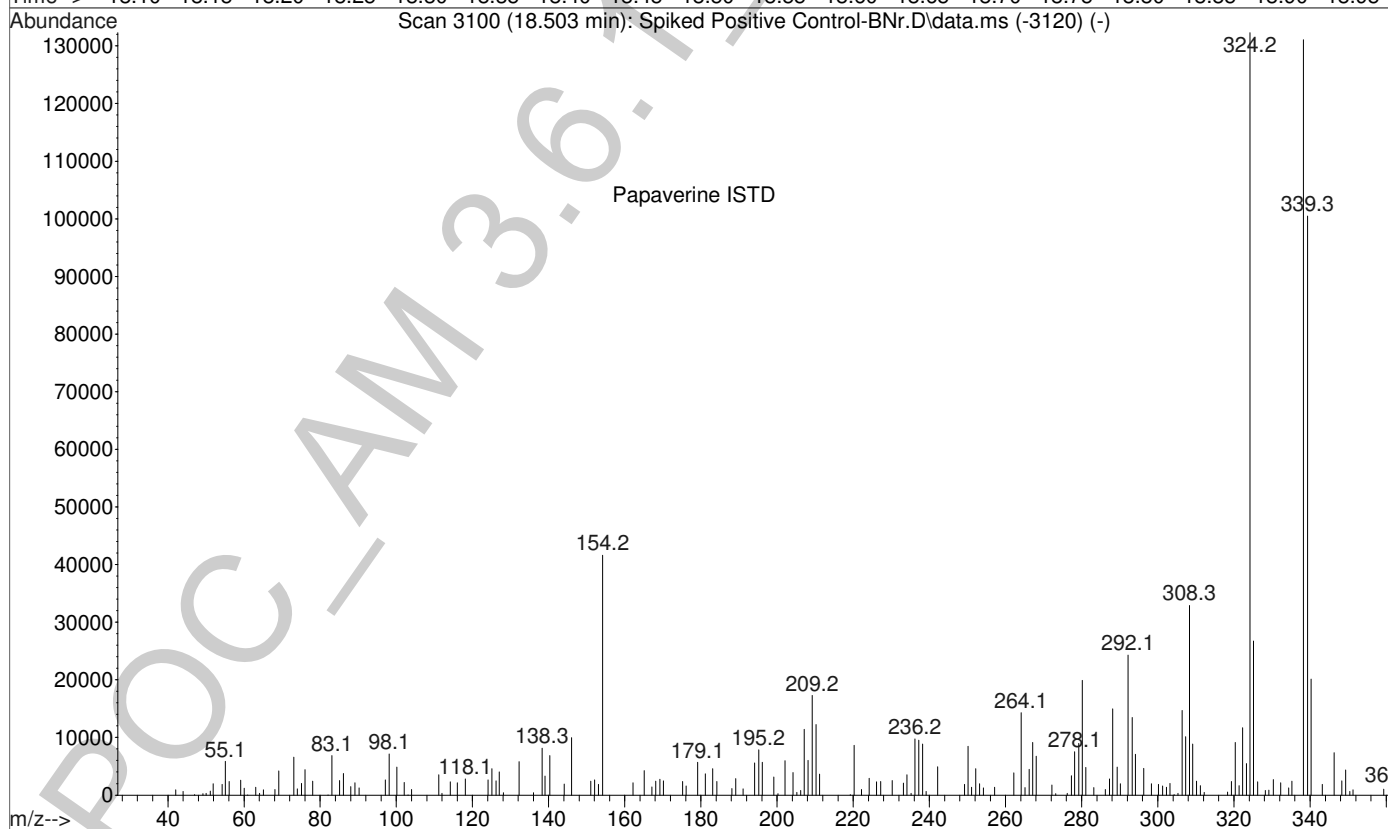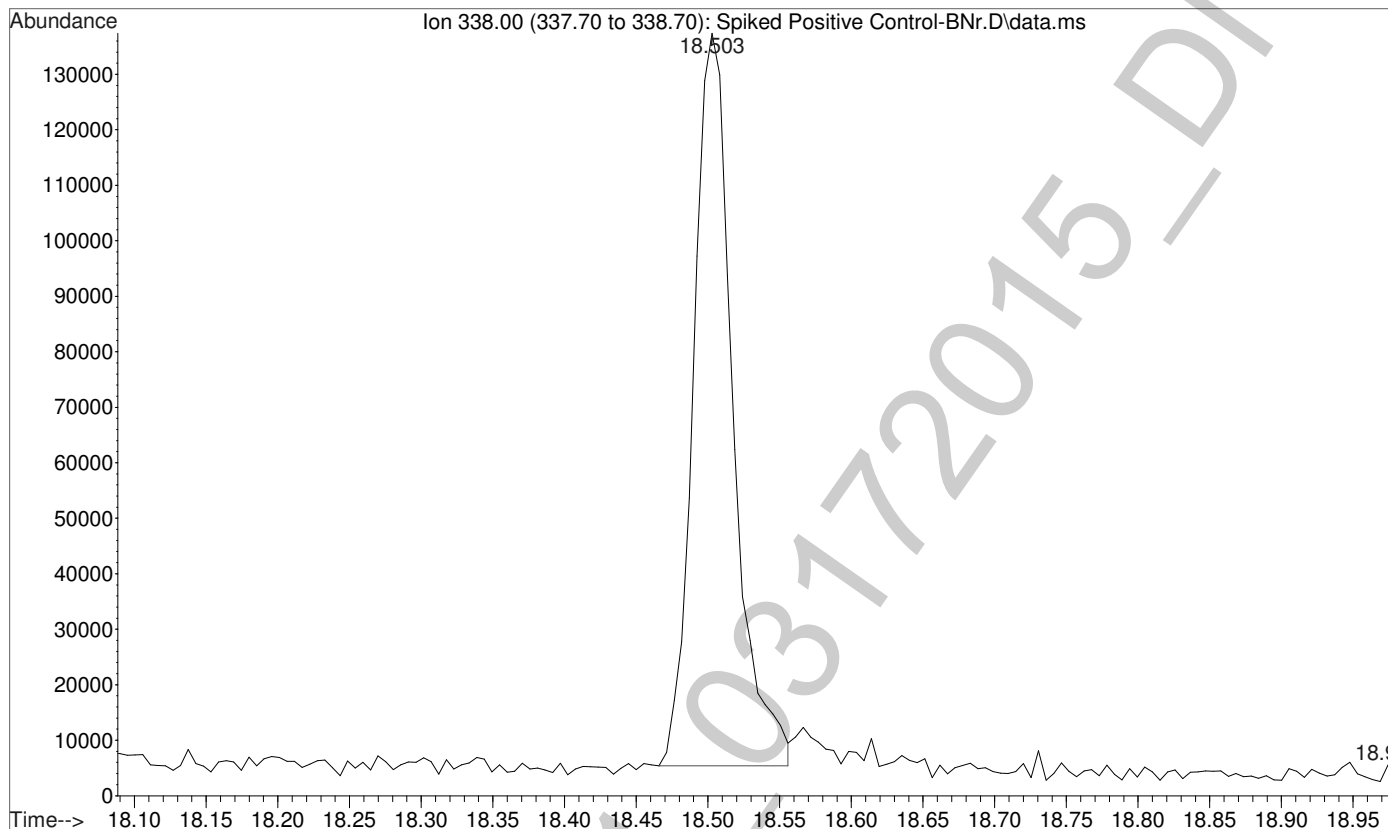



File :C:\gcms\1\data\Blood\031715BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 17 Mar 2015 20:18 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

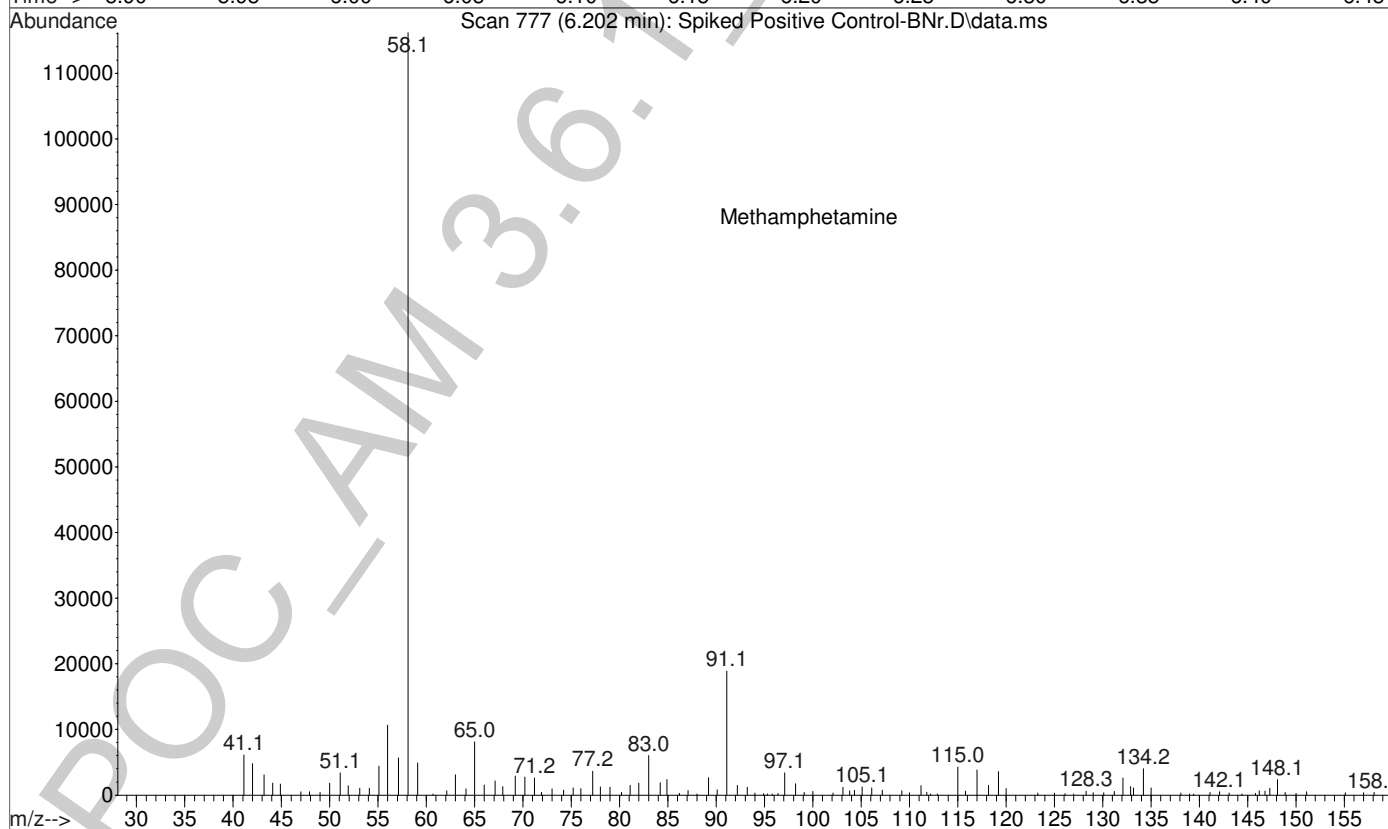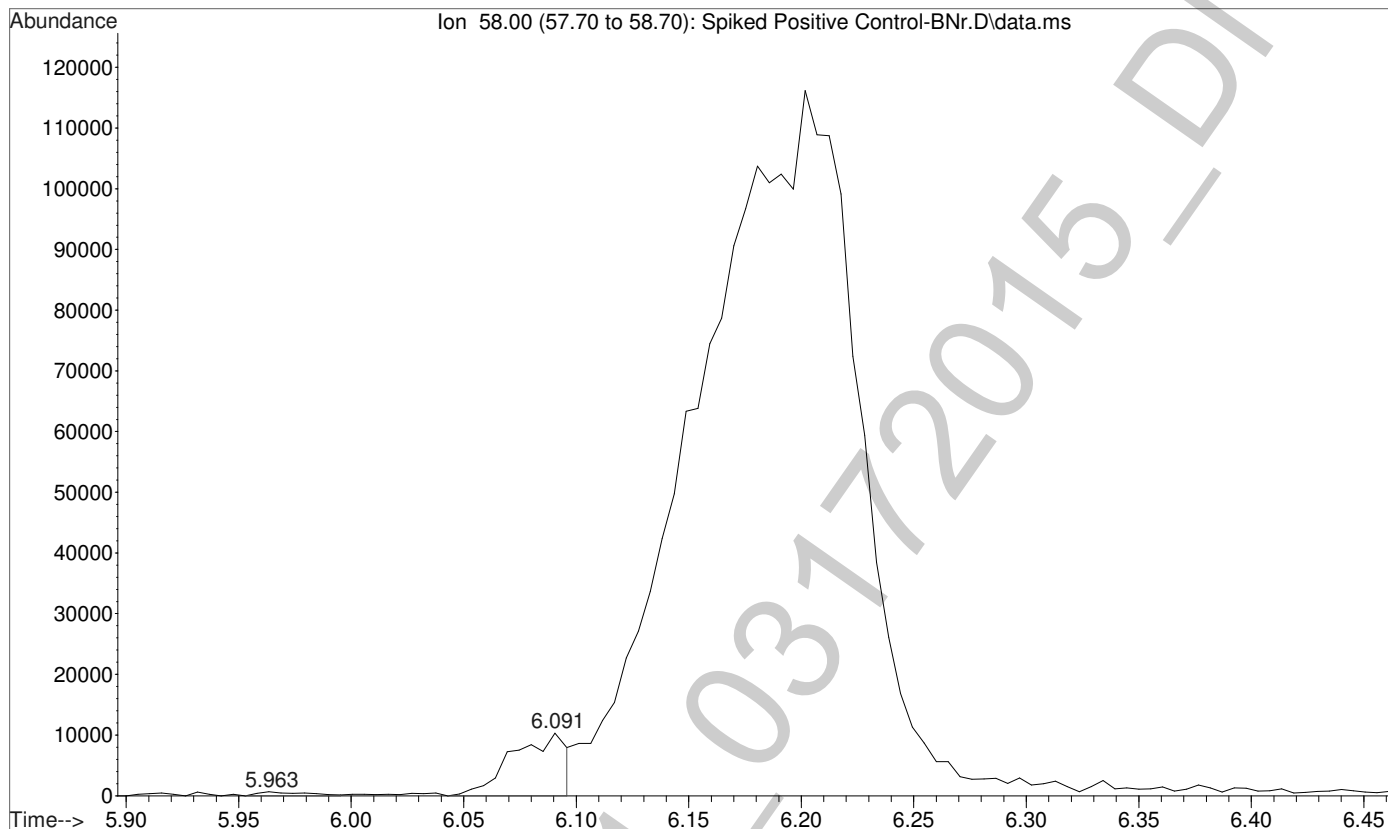



File :C:\gcms\1\data\Blood\031715BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 17 Mar 2015 20:18 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

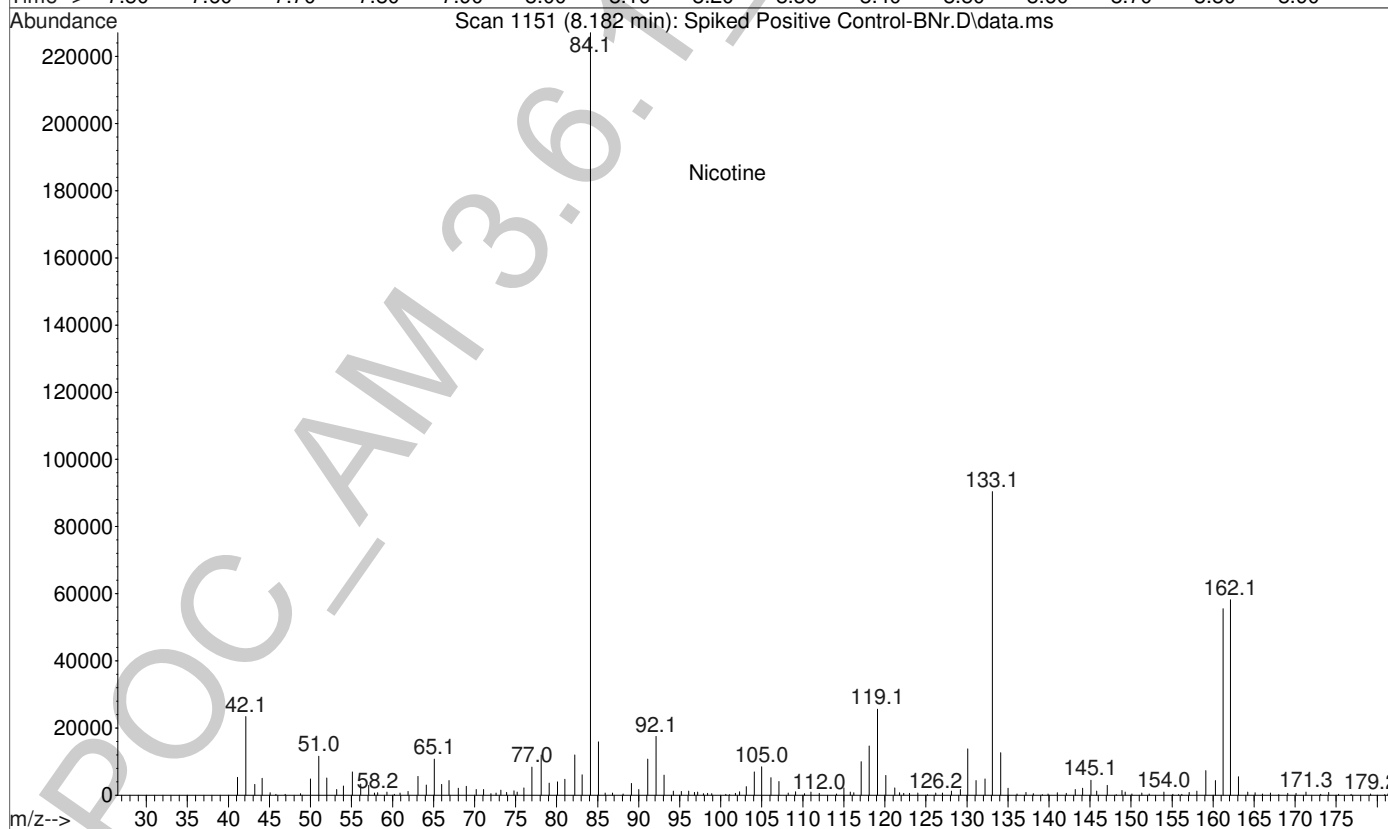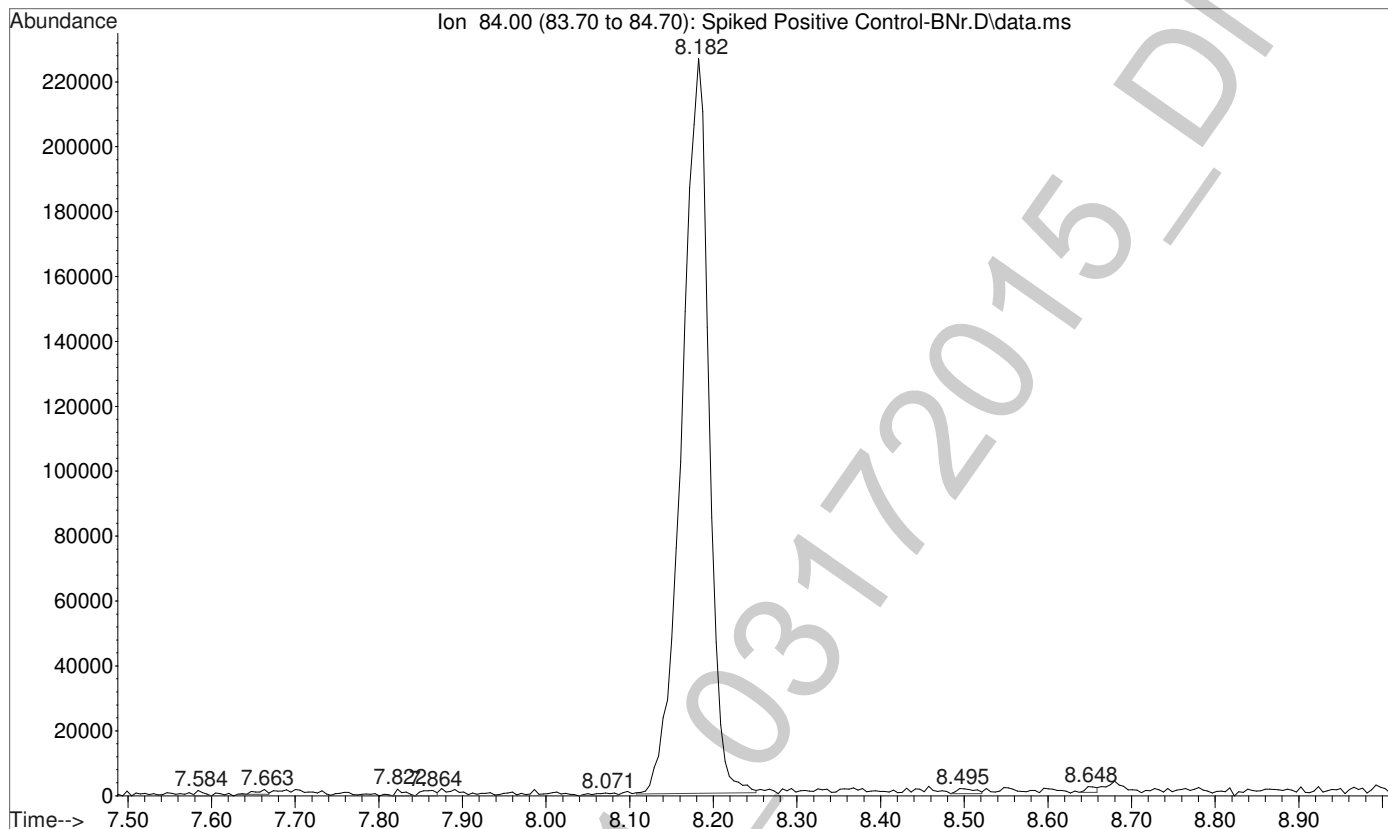



File :C:\gcms\1\data\Blood\031715BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 17 Mar 2015 20:18 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

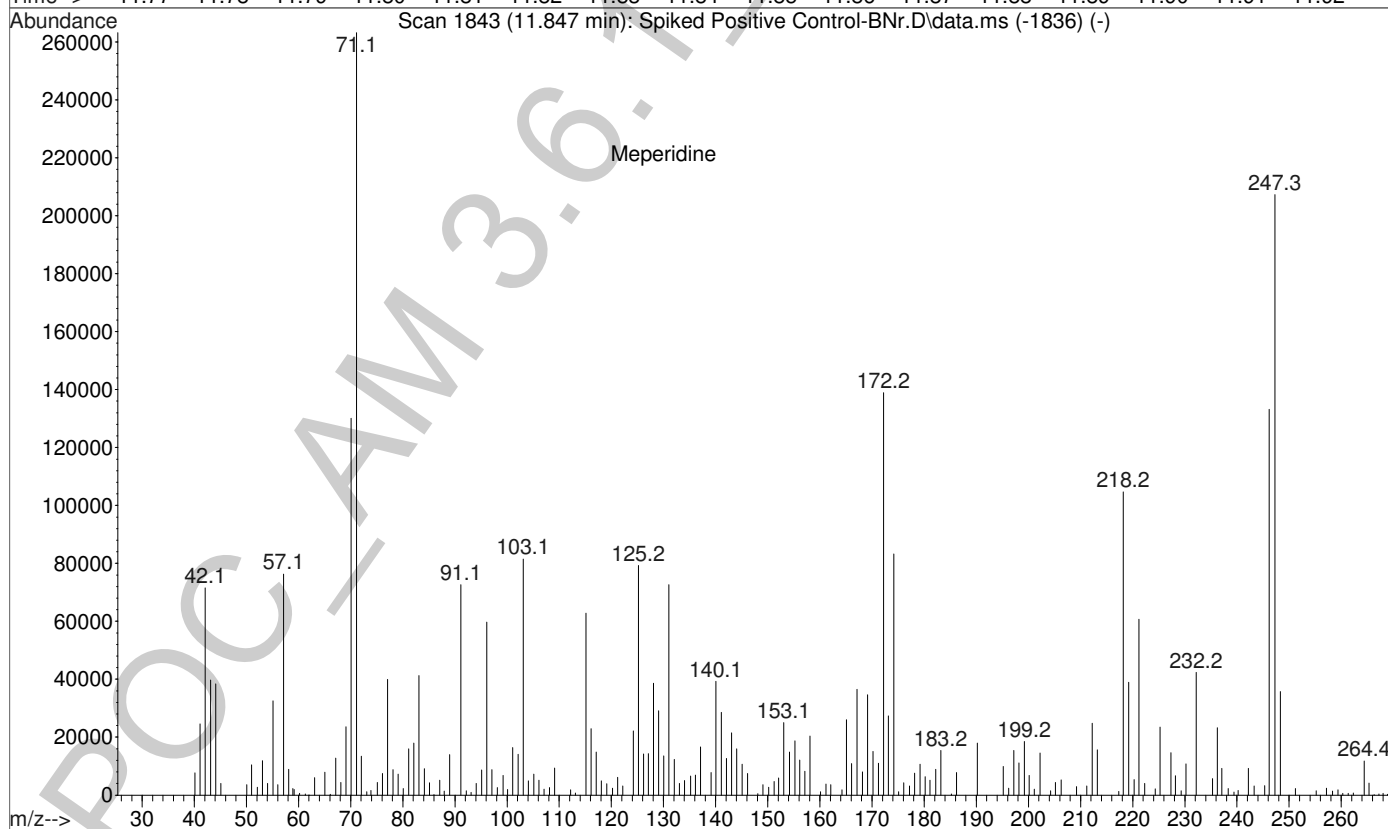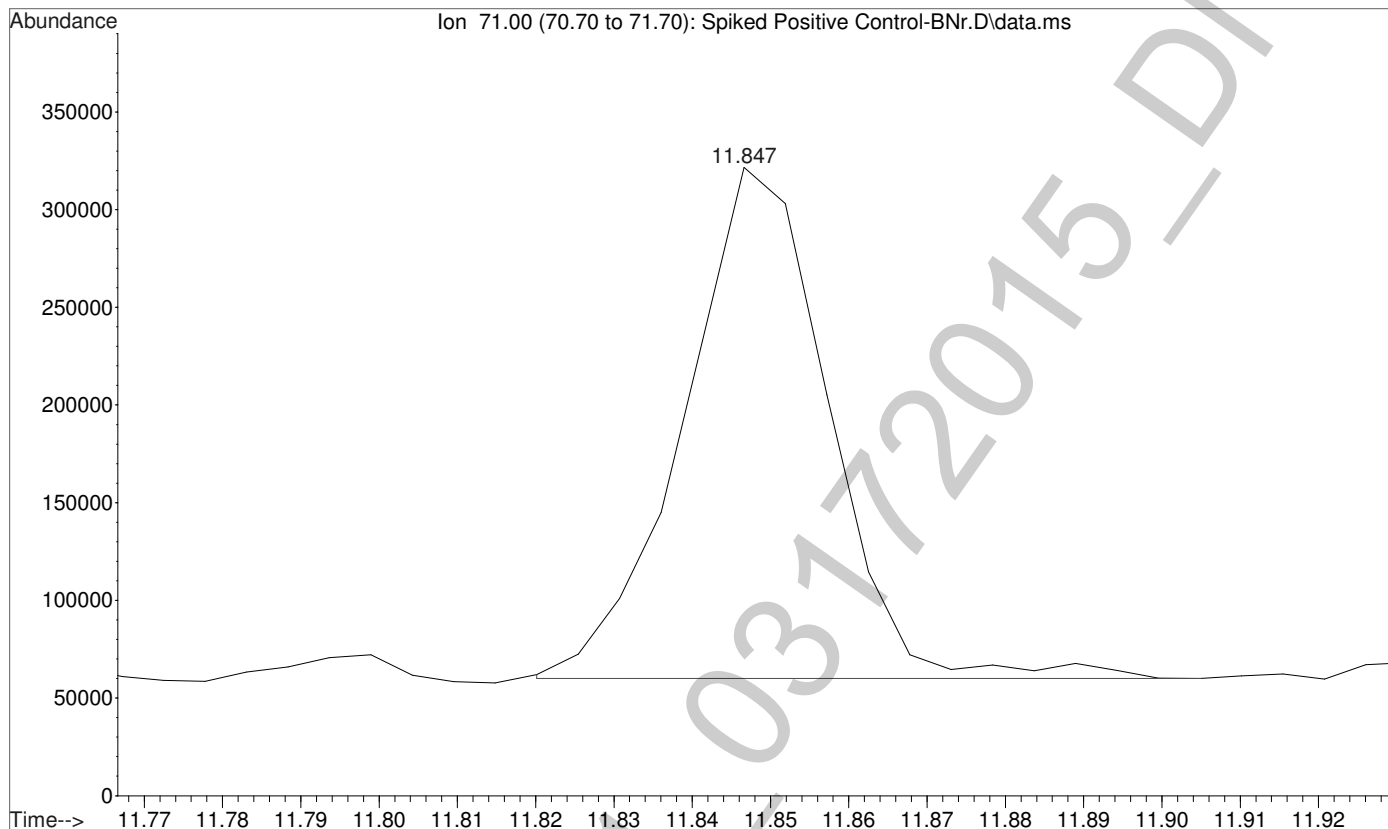



File :C:\gcms\1\data\Blood\031715BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 17 Mar 2015 20:18 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

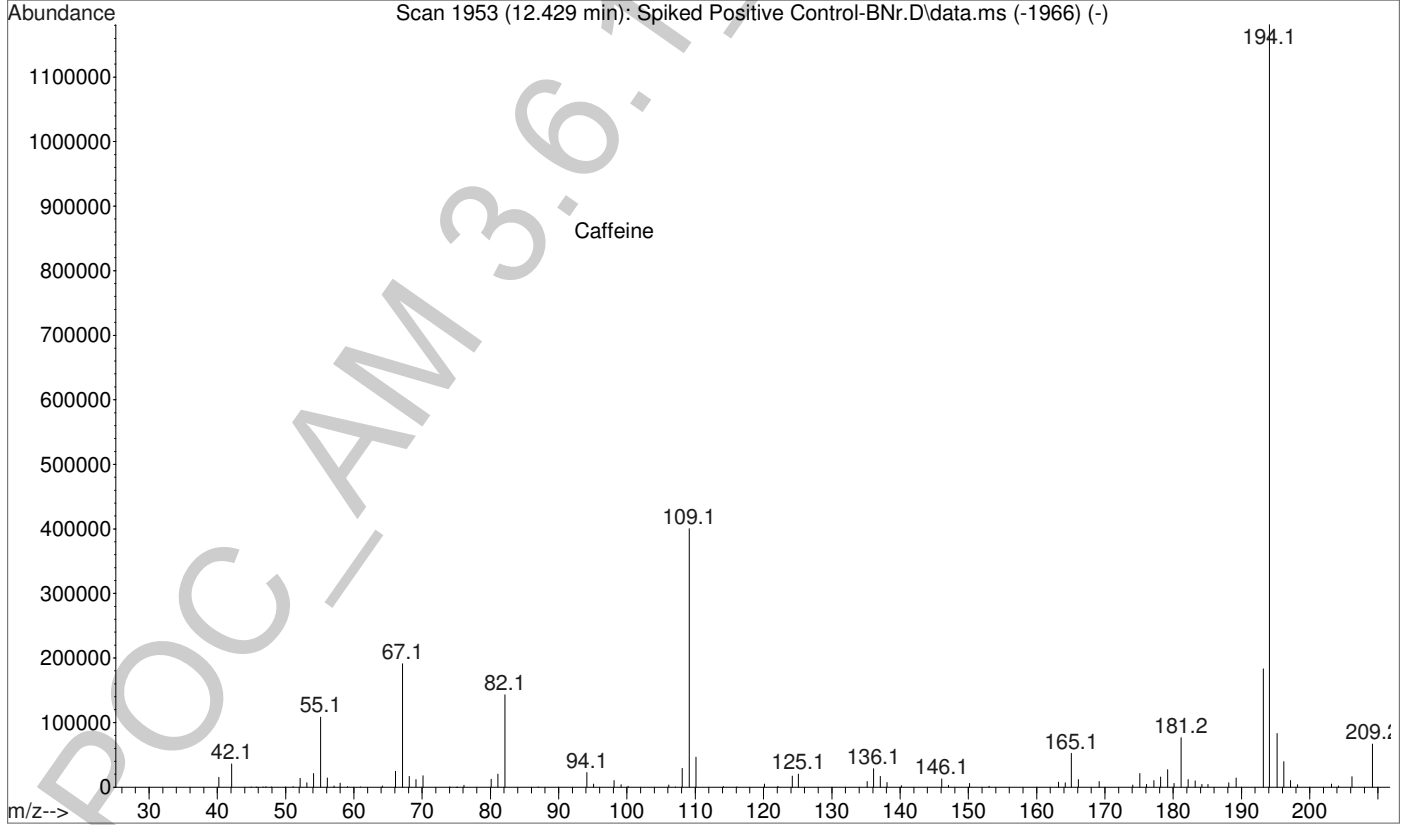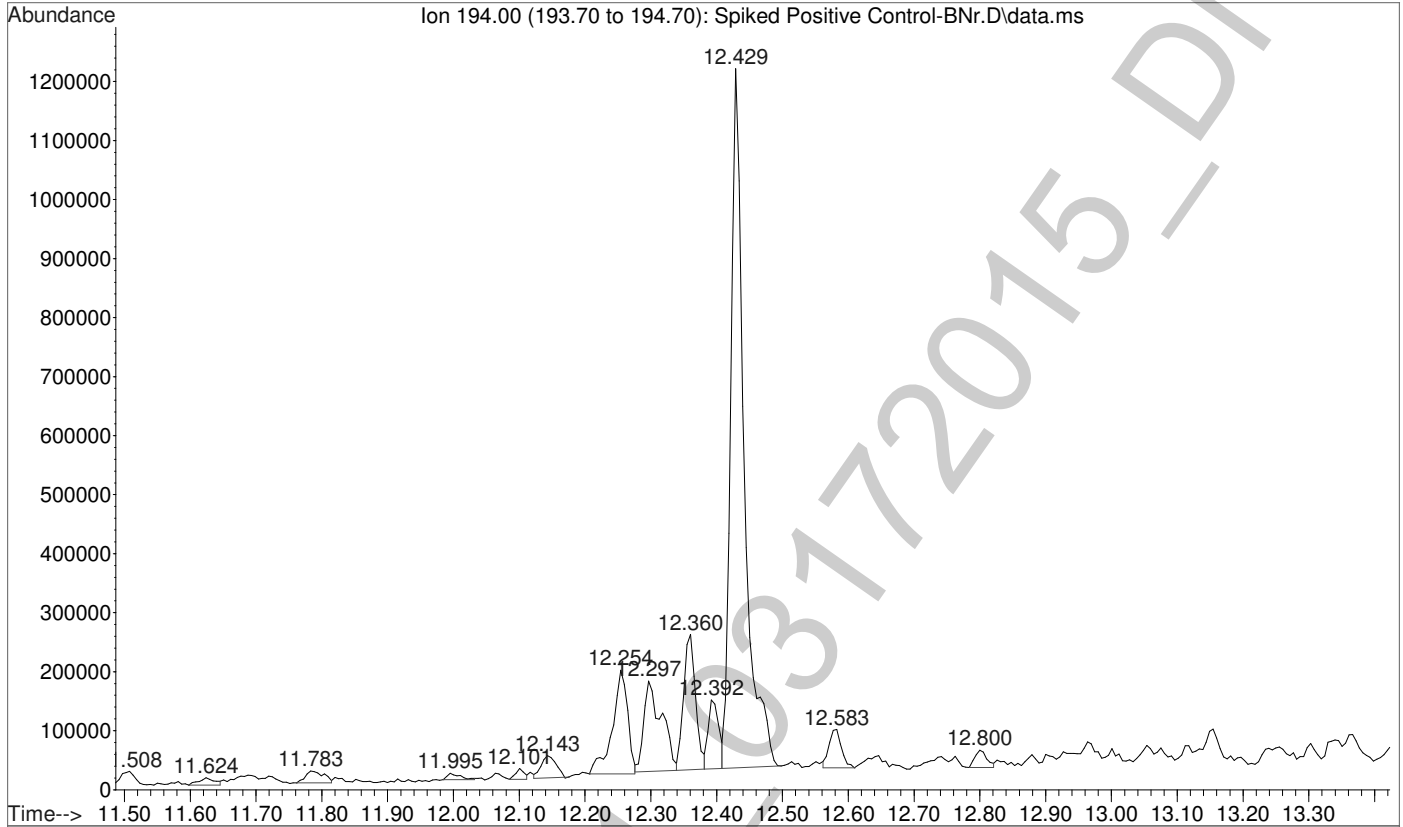



File :C:\gcms\1\data\Blood\031715BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 17 Mar 2015 20:18 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

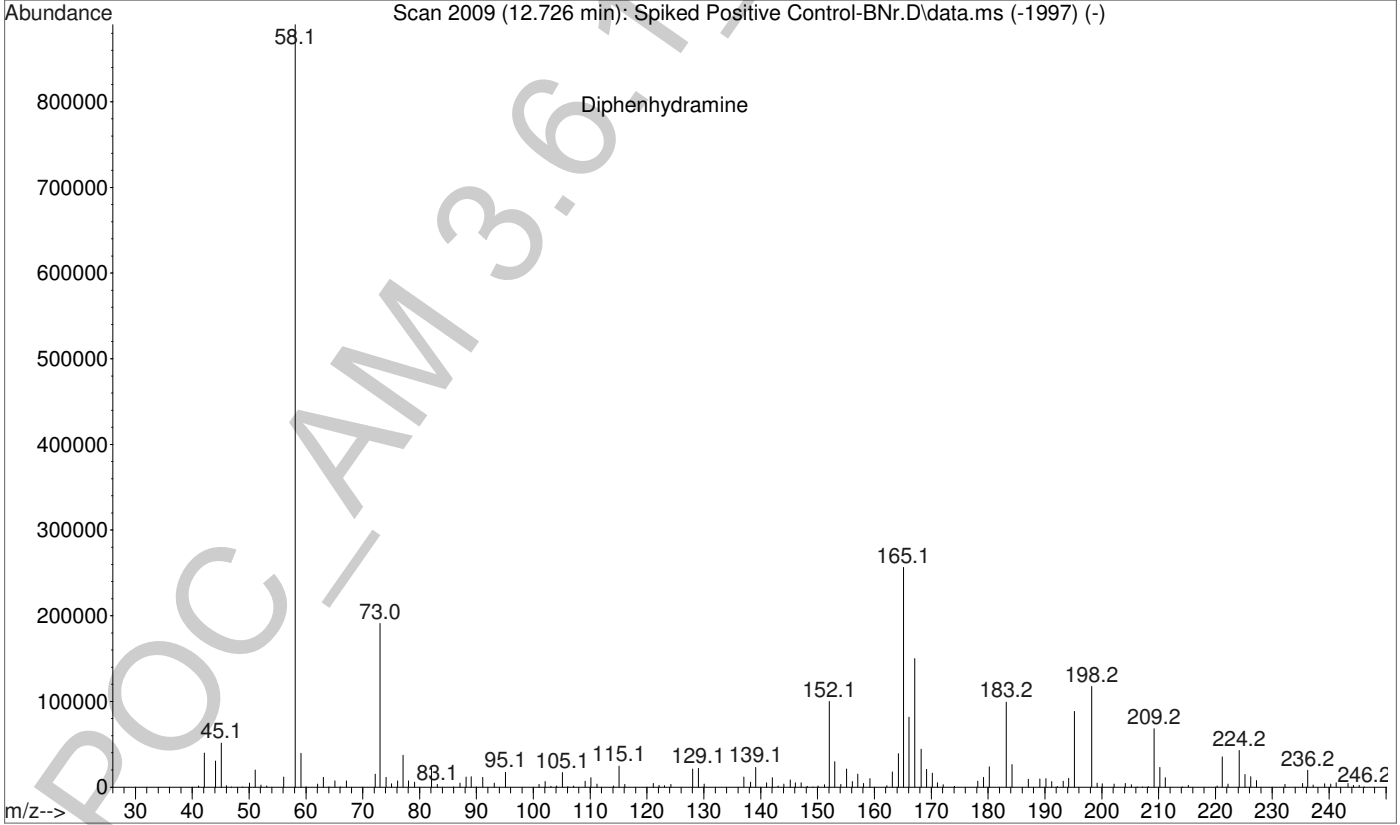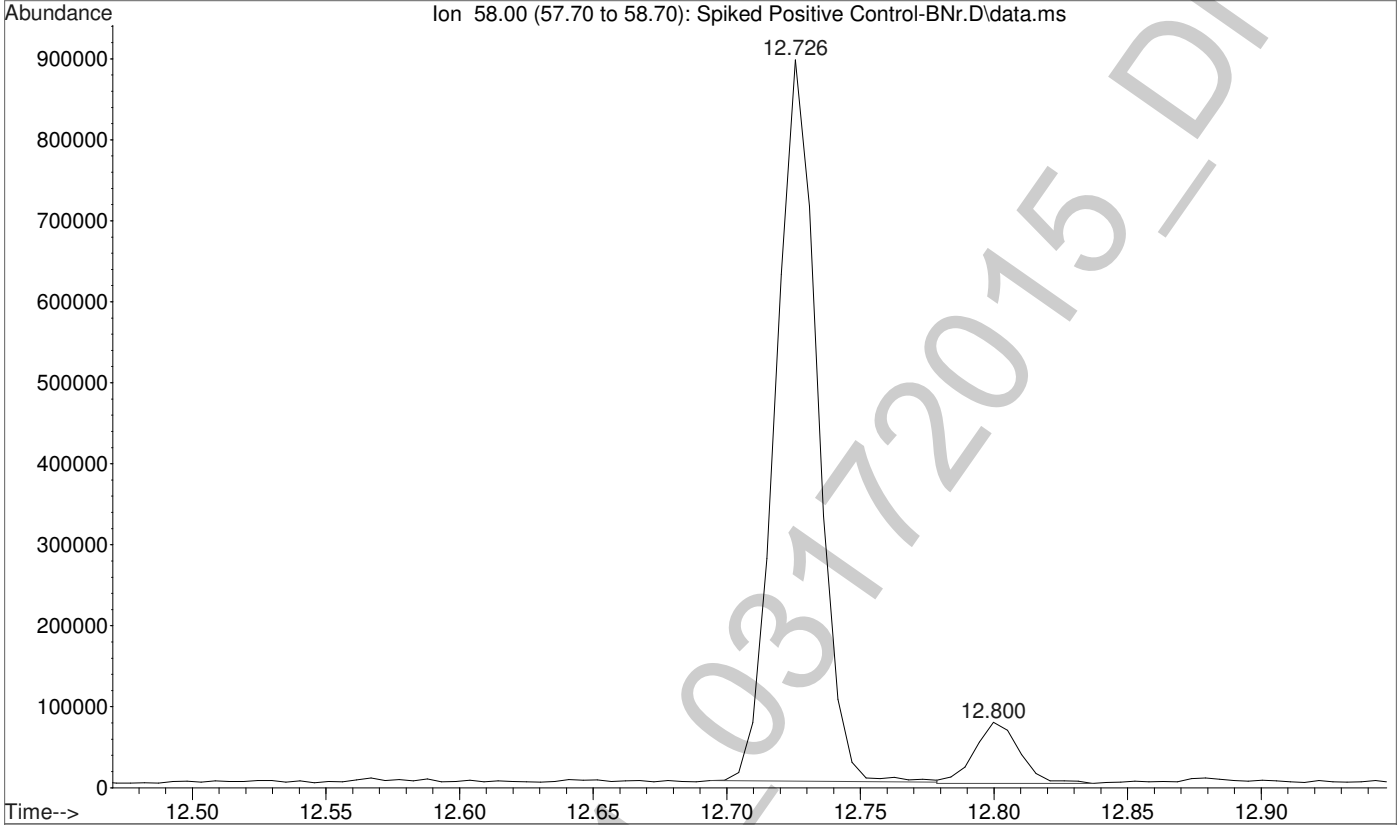



File :C:\gcms\1\data\Blood\031715BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 17 Mar 2015 20:18 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

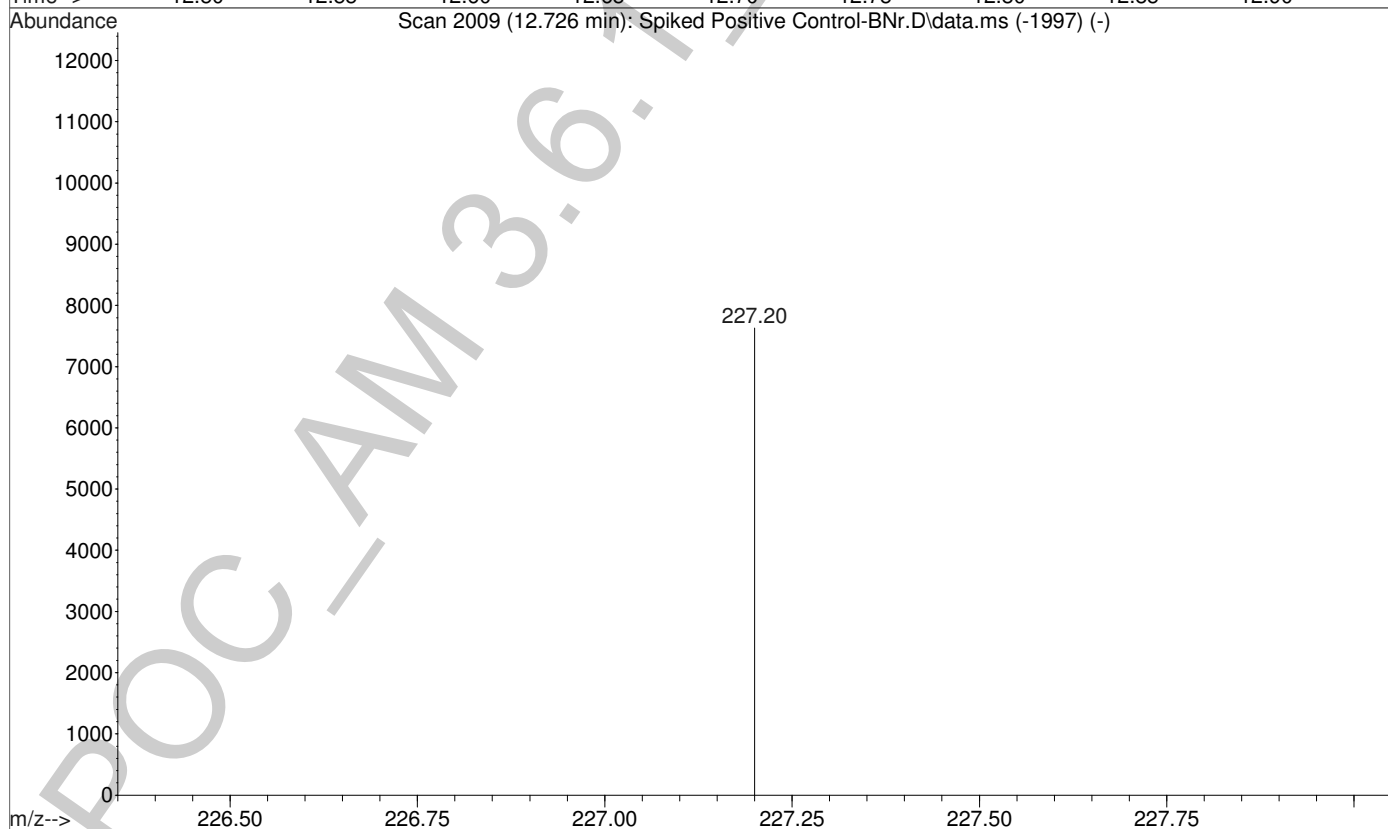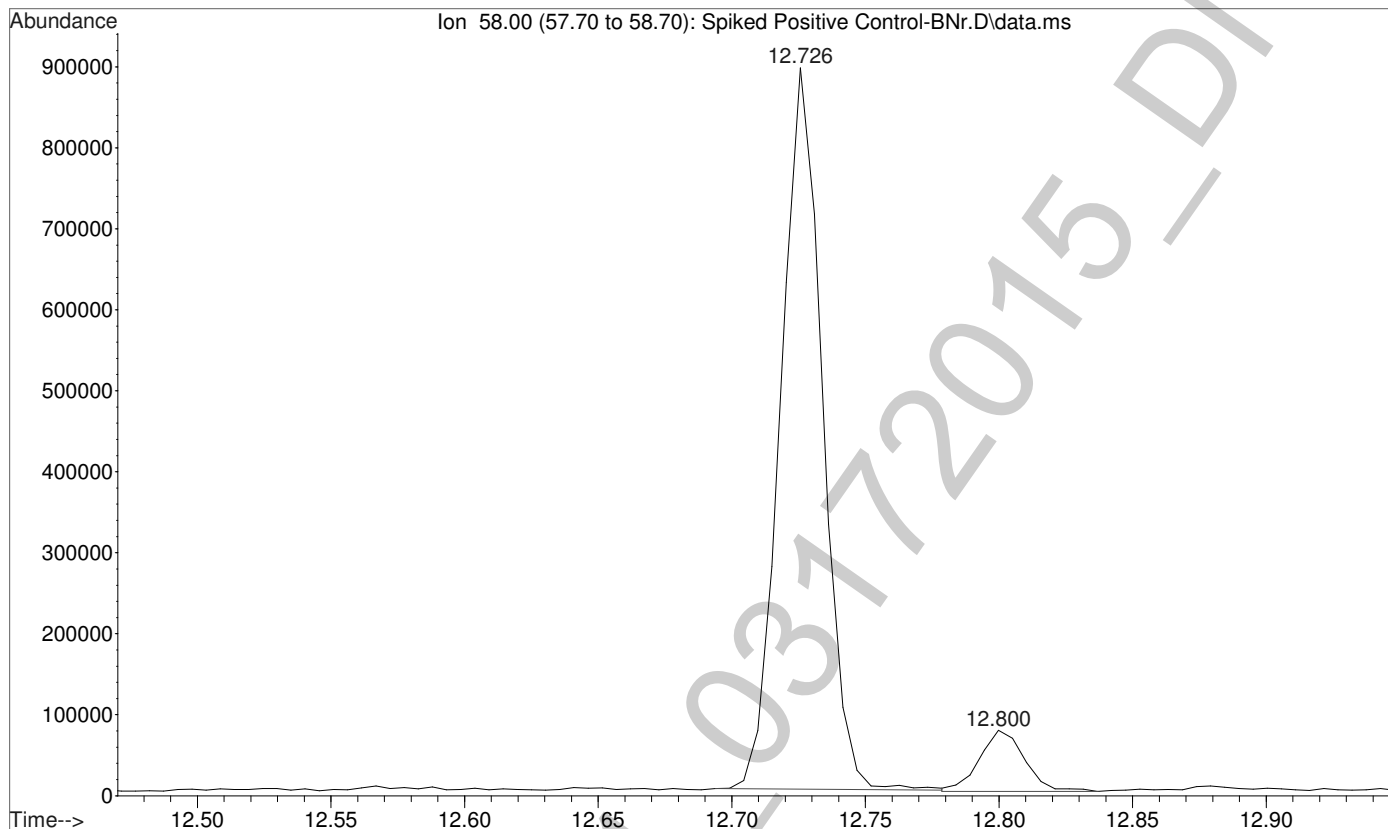



File :C:\gcms\1\data\Blood\031715BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 17 Mar 2015 20:18 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

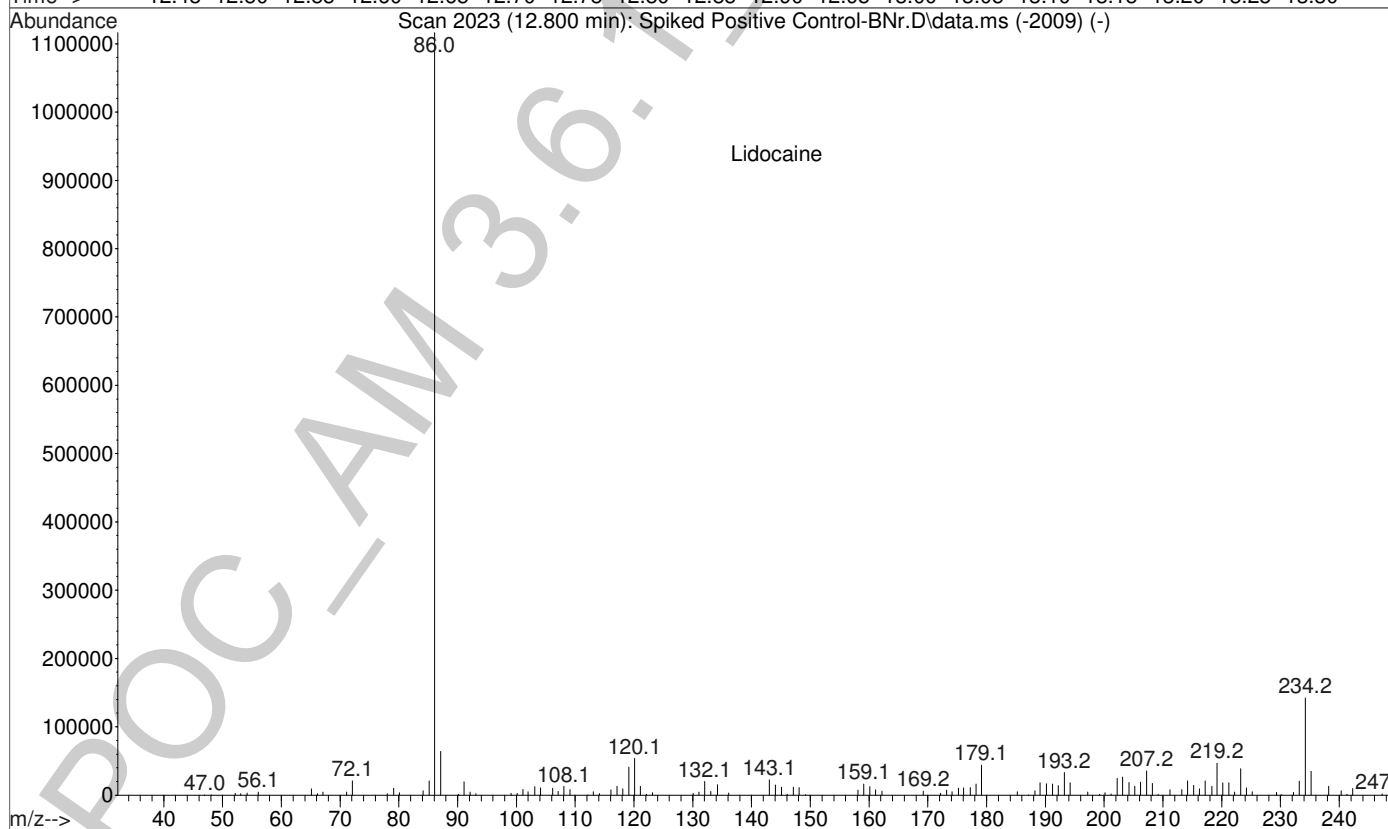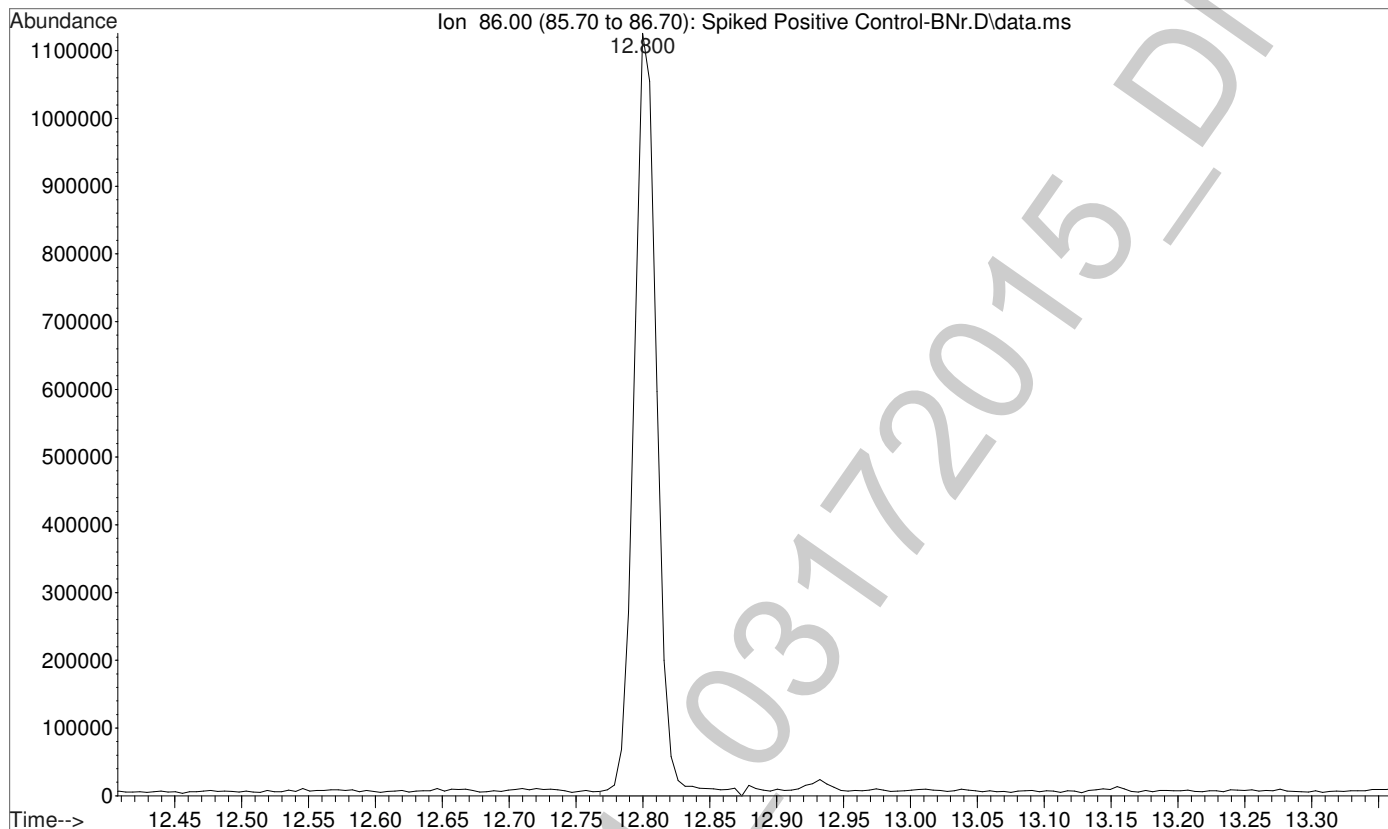



File :C:\gcms\1\data\Blood\031715BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 17 Mar 2015 20:18 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

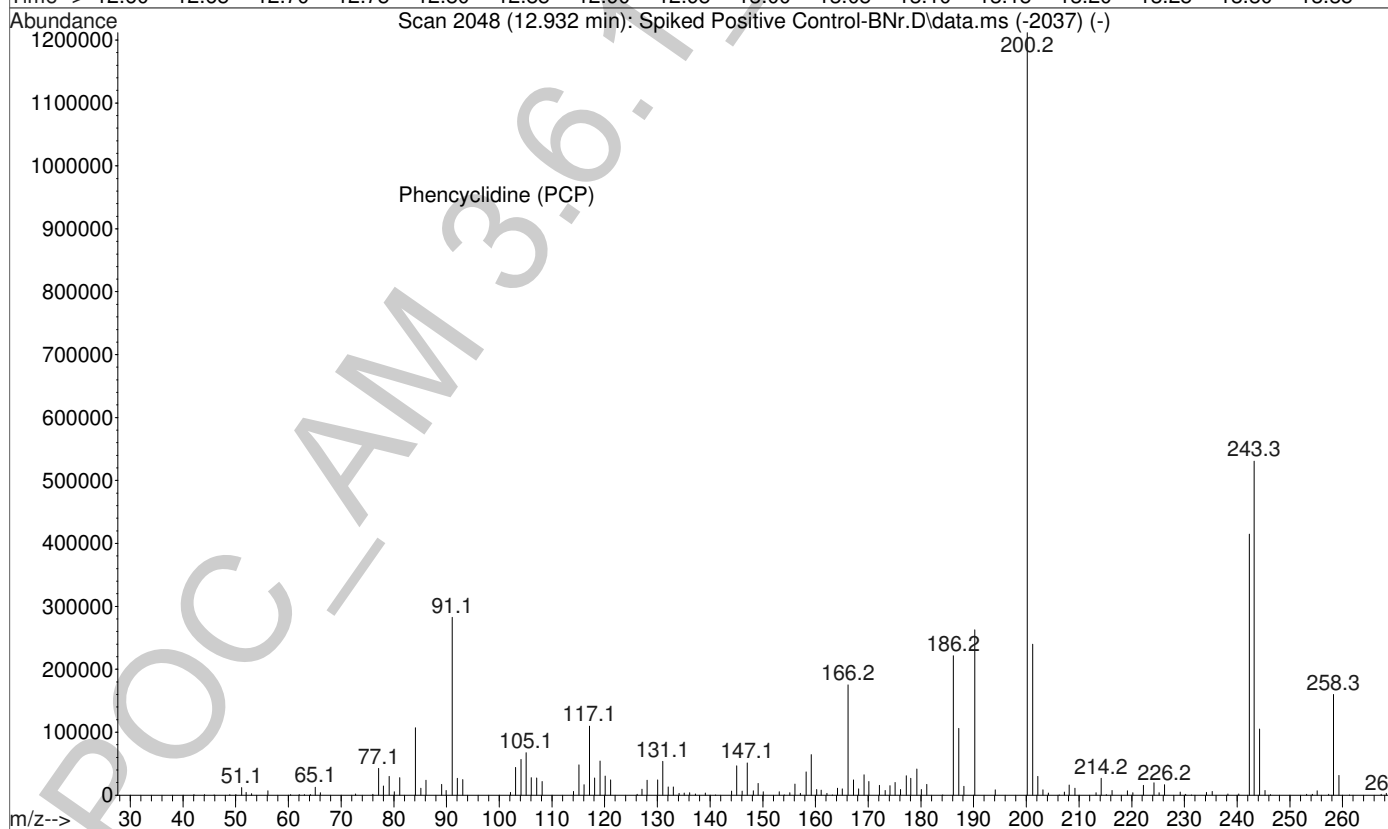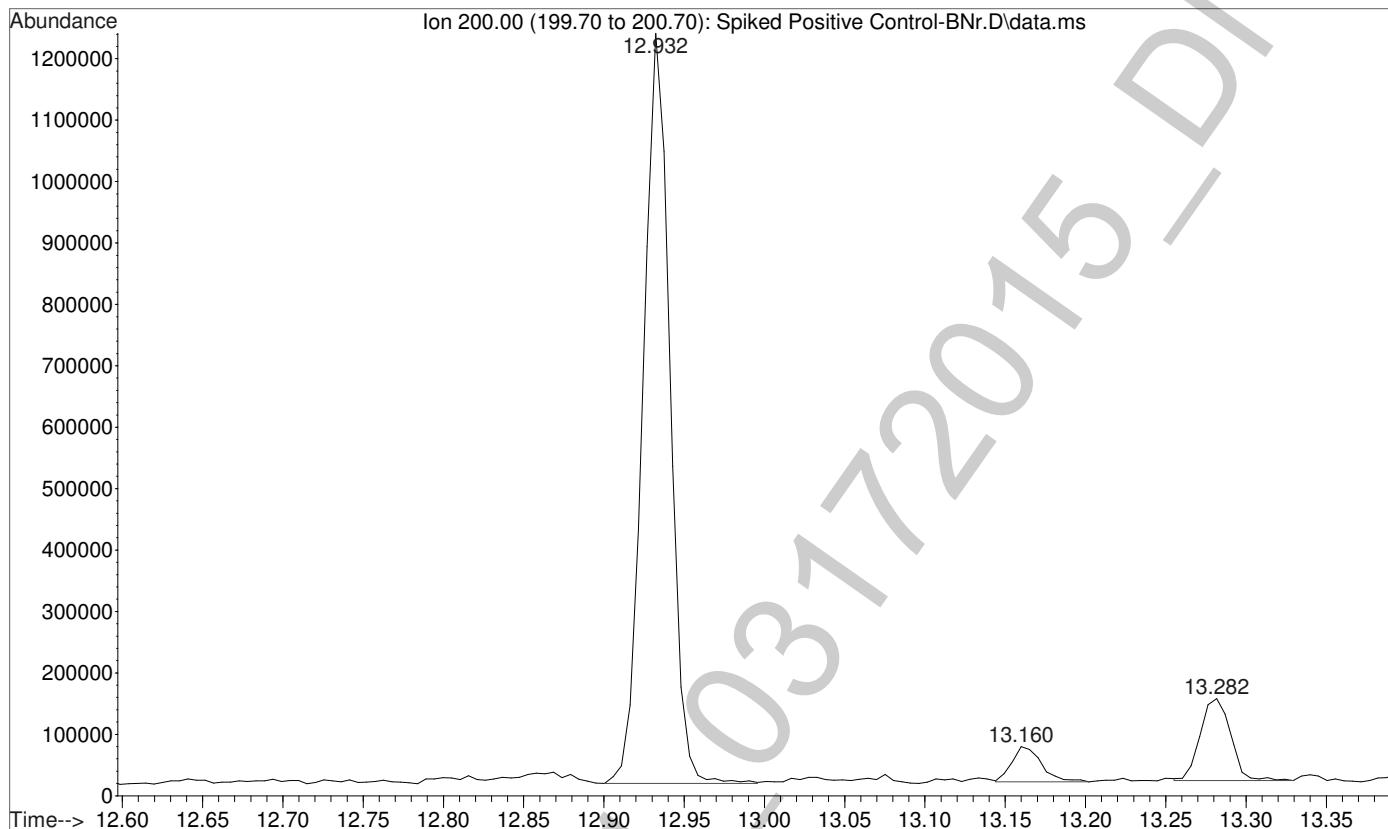



File :C:\gcms\1\data\Blood\031715BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 17 Mar 2015 20:18 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

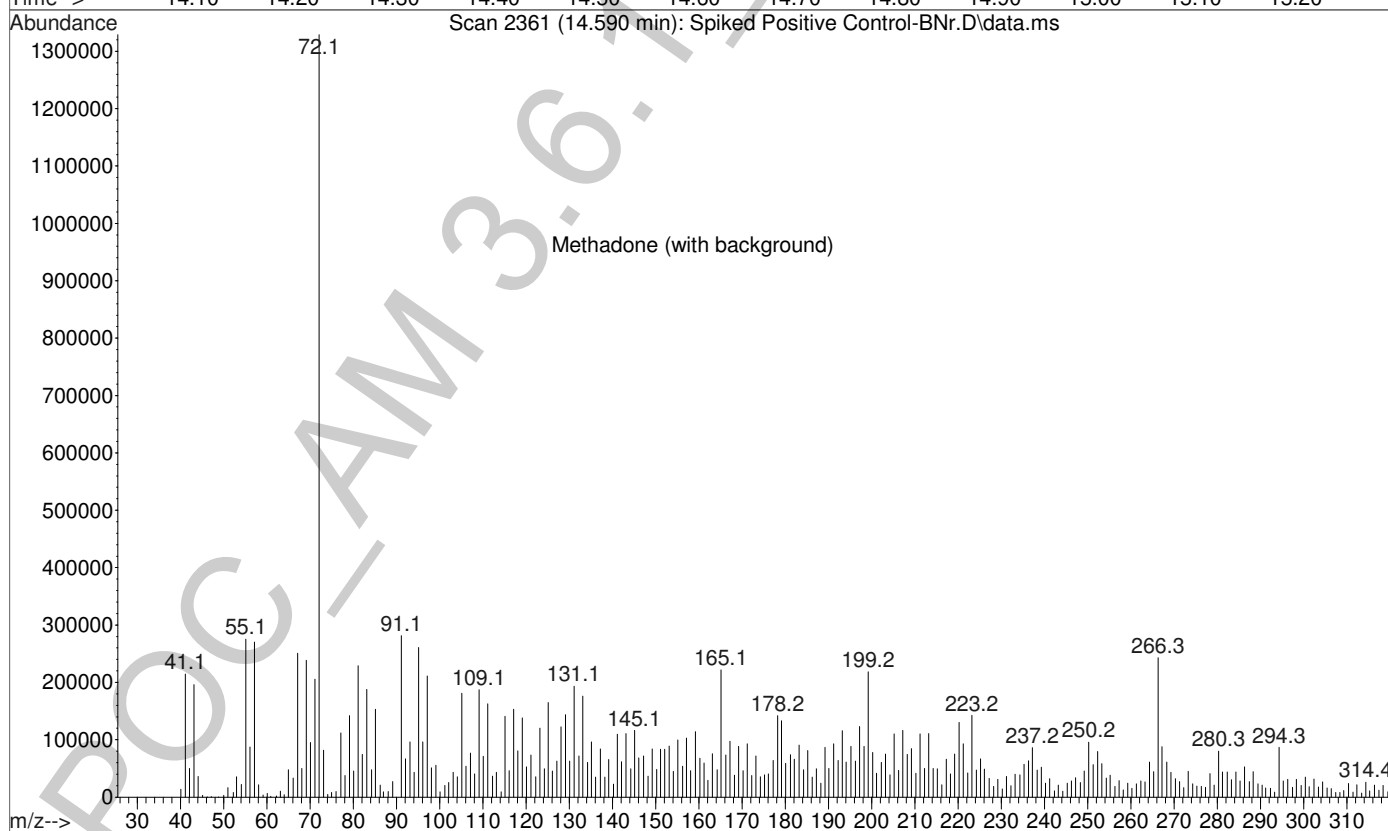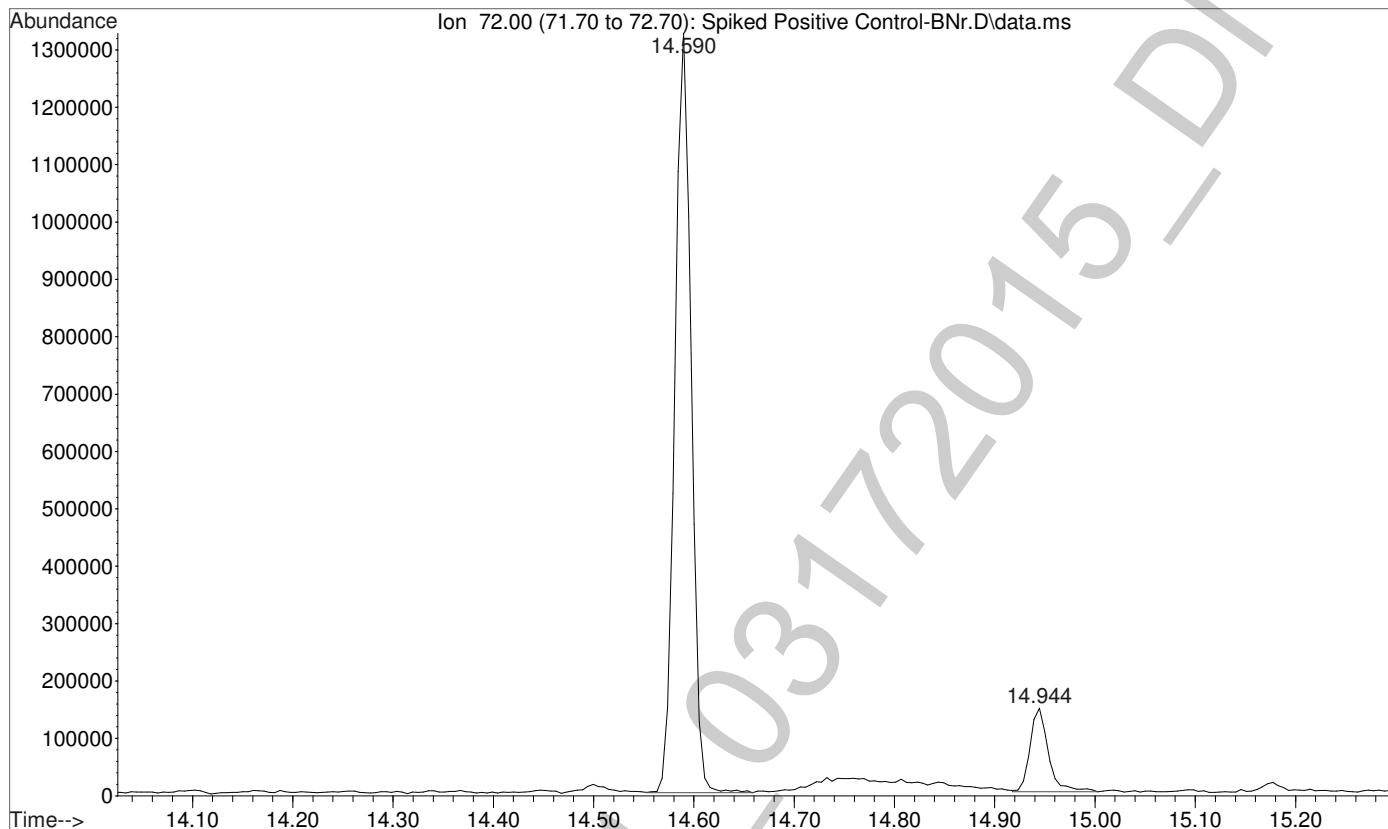



File :C:\gcms\1\data\Blood\031715BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 17 Mar 2015 20:18 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

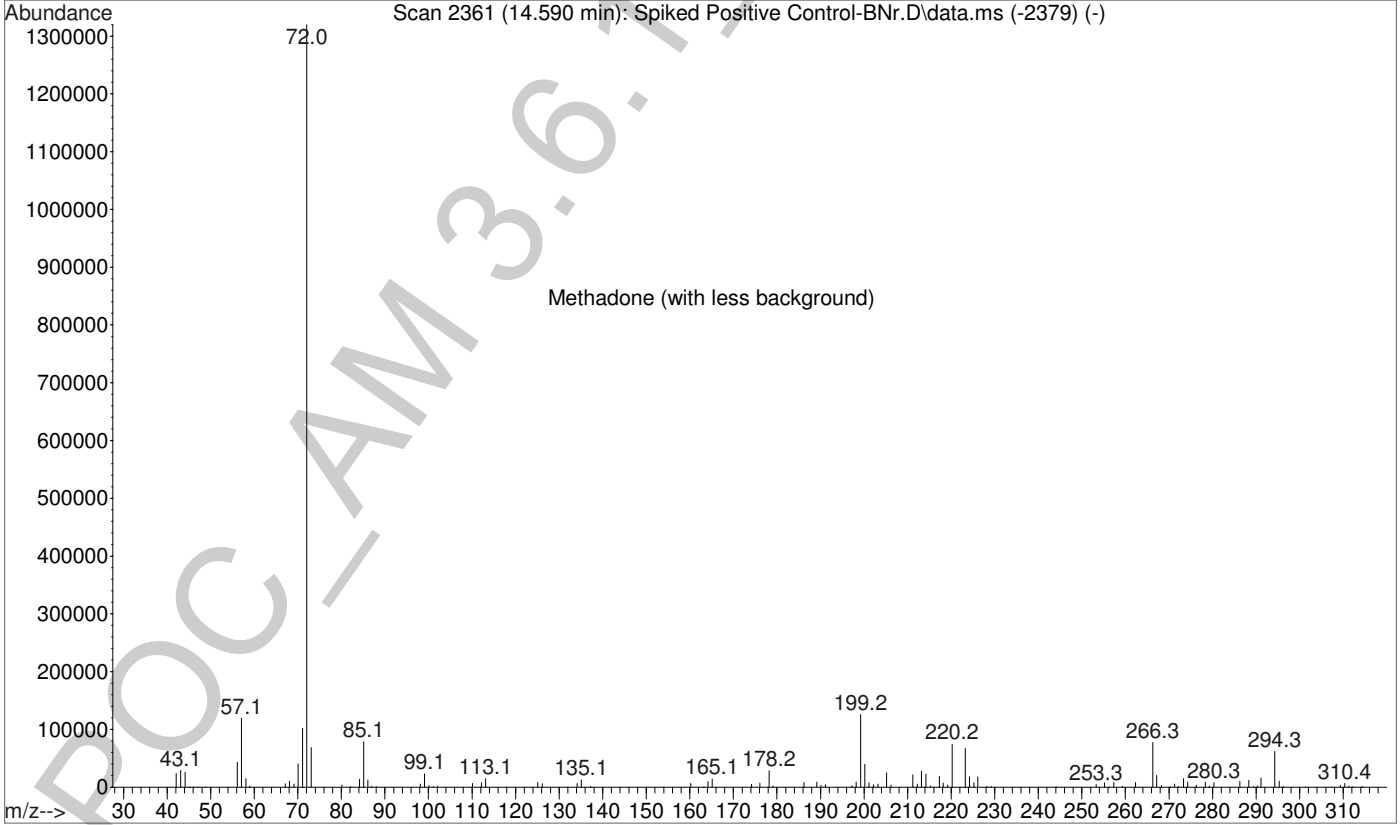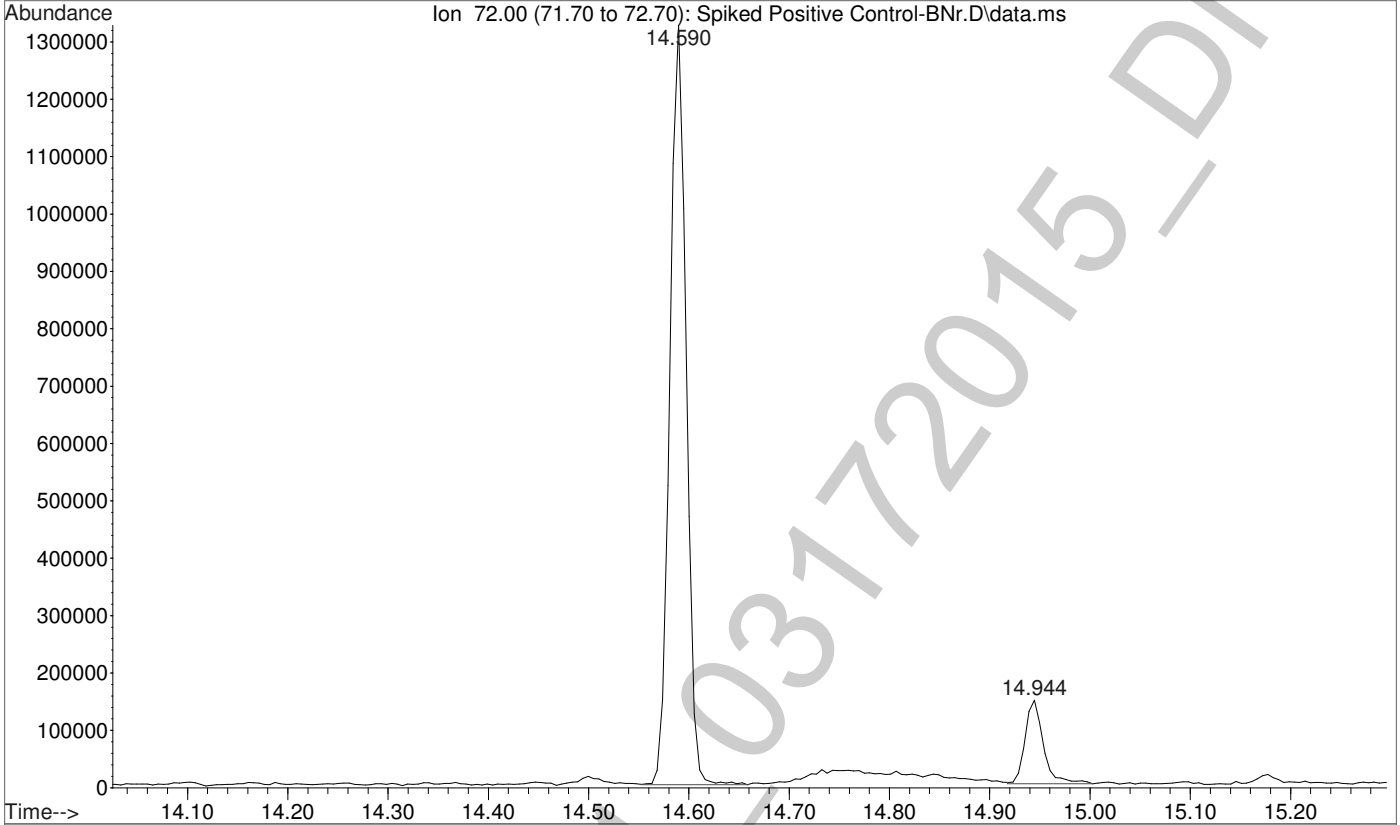



File :C:\gcms\1\data\Blood\031715BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 17 Mar 2015 20:18 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

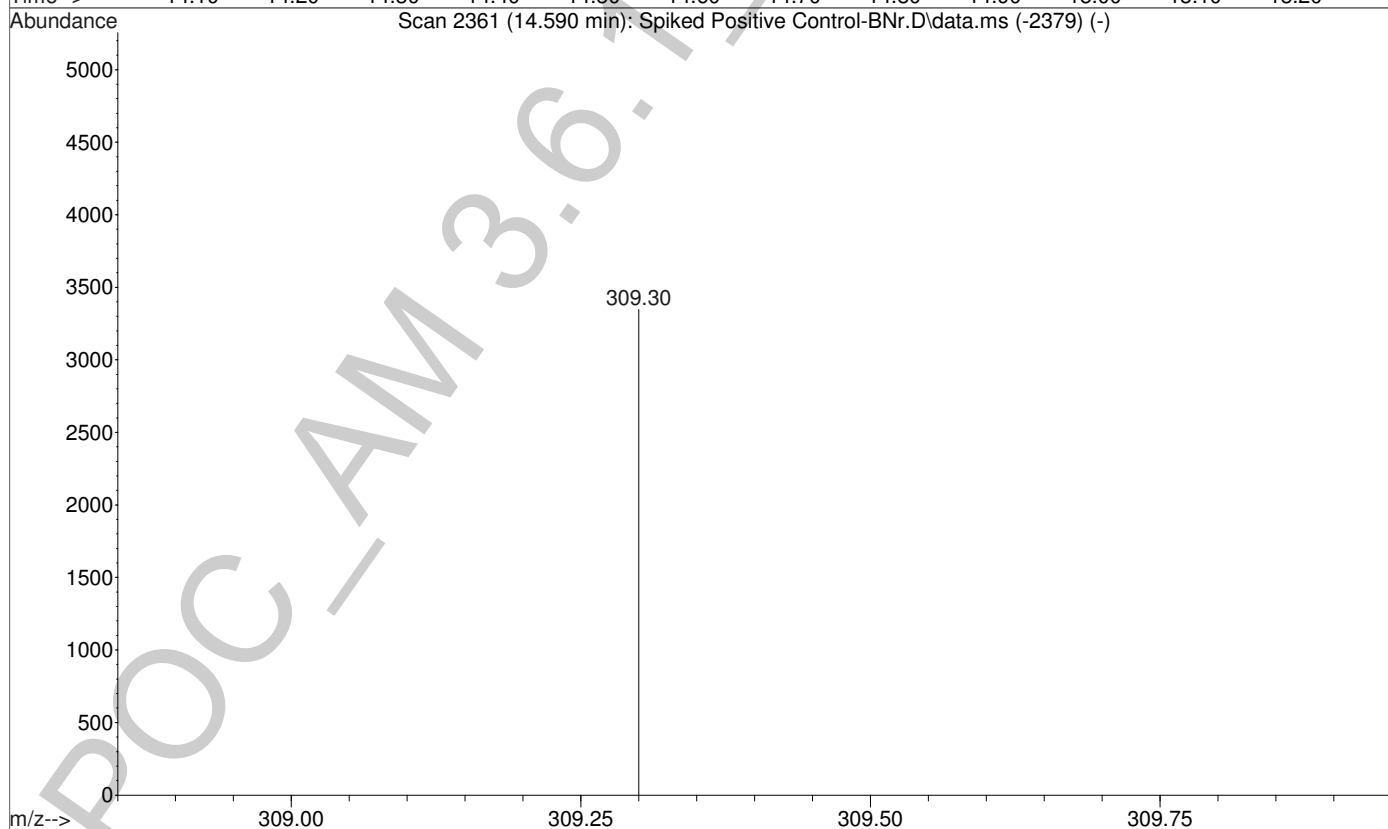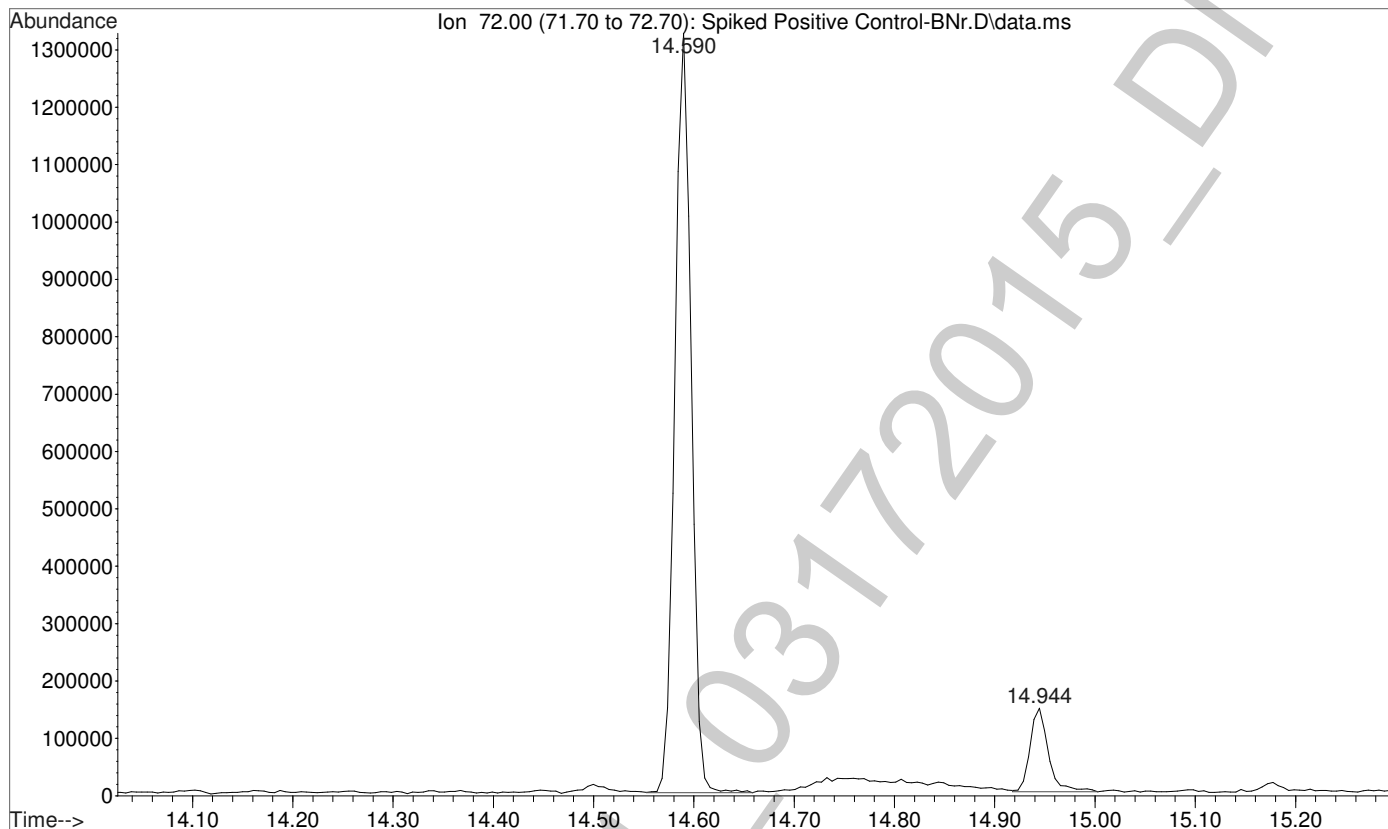



File :C:\gcms\1\data\Blood\031715BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 17 Mar 2015 20:18 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

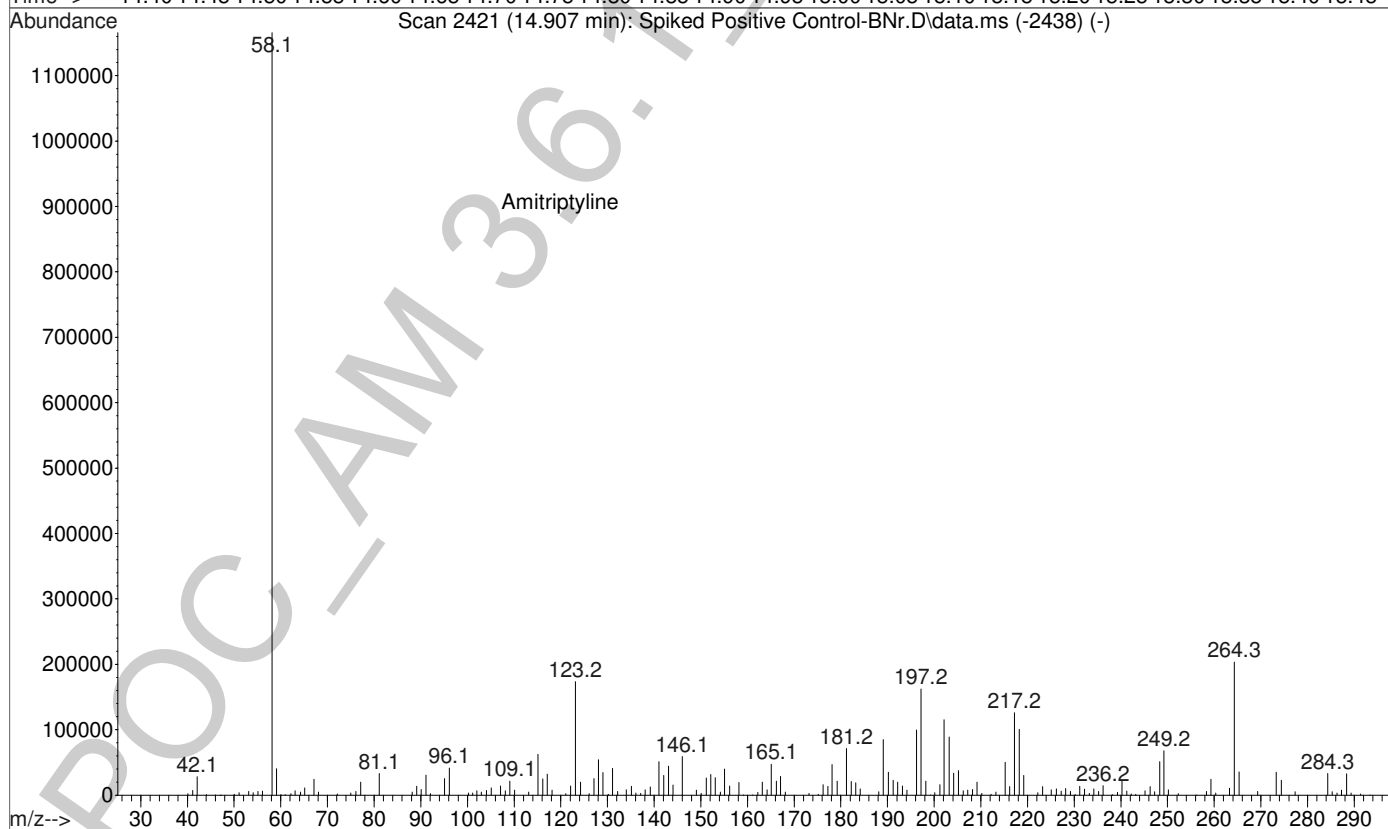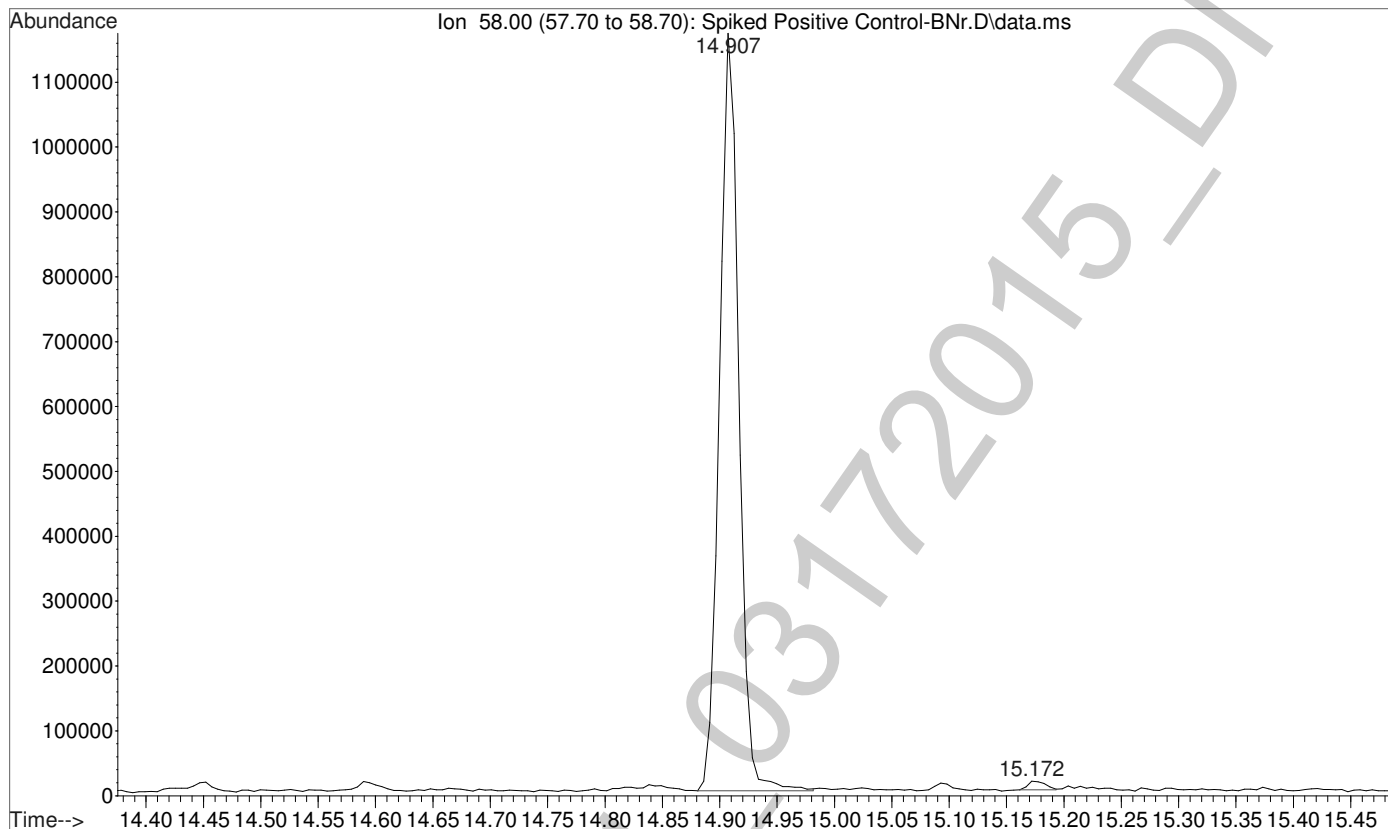



File :C:\gcms\1\data\Blood\031715BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 17 Mar 2015 20:18 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

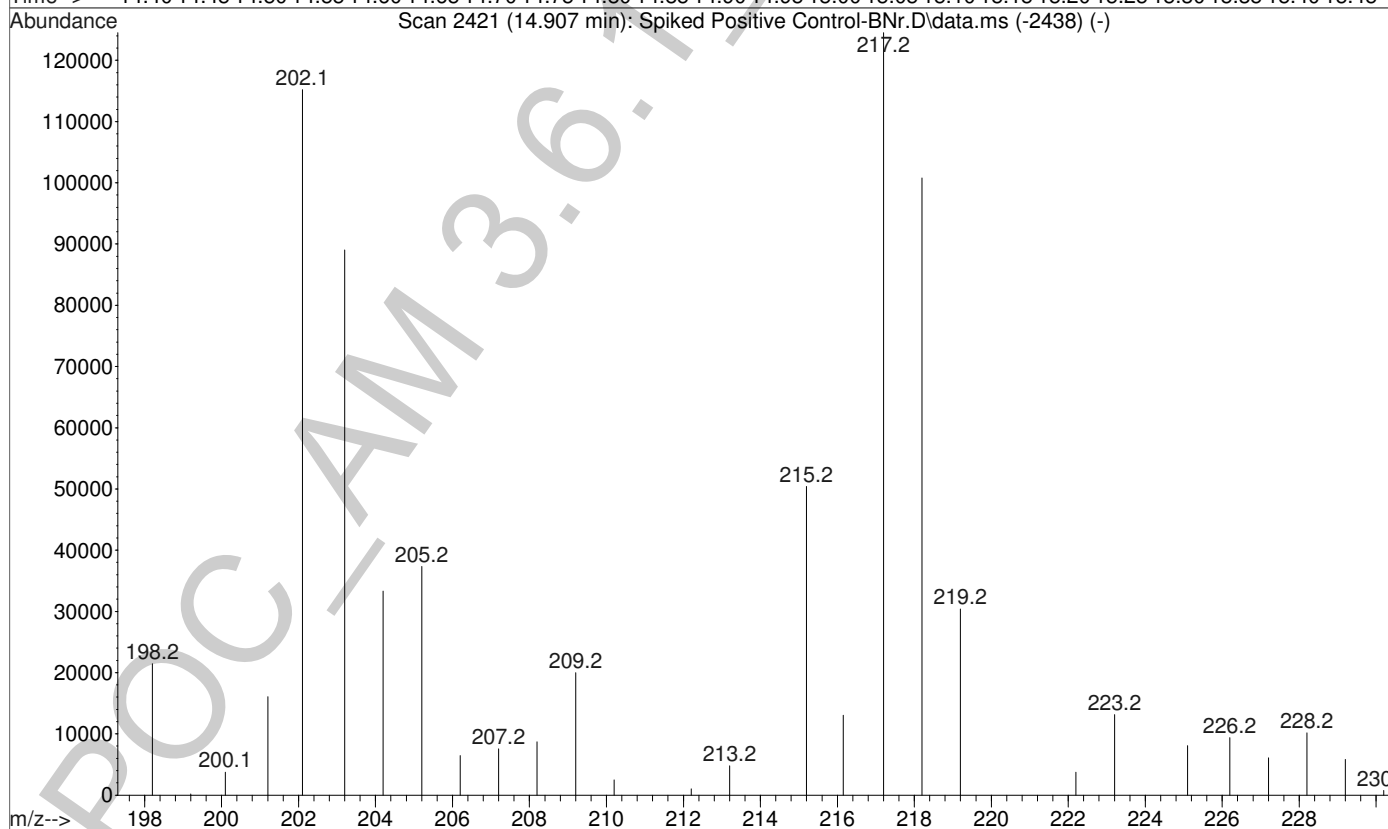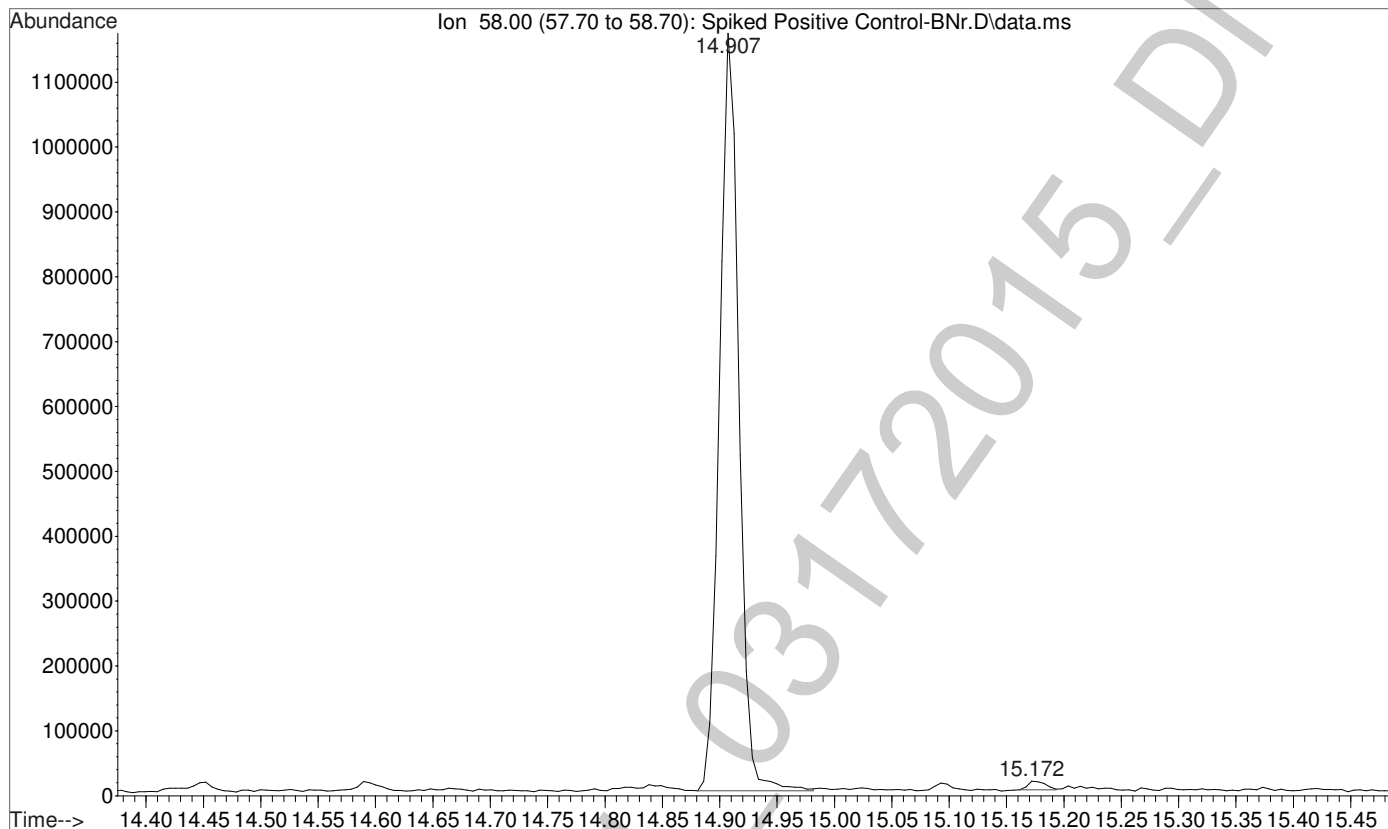



File :C:\gcms\1\data\Blood\031715BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 17 Mar 2015 20:18 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

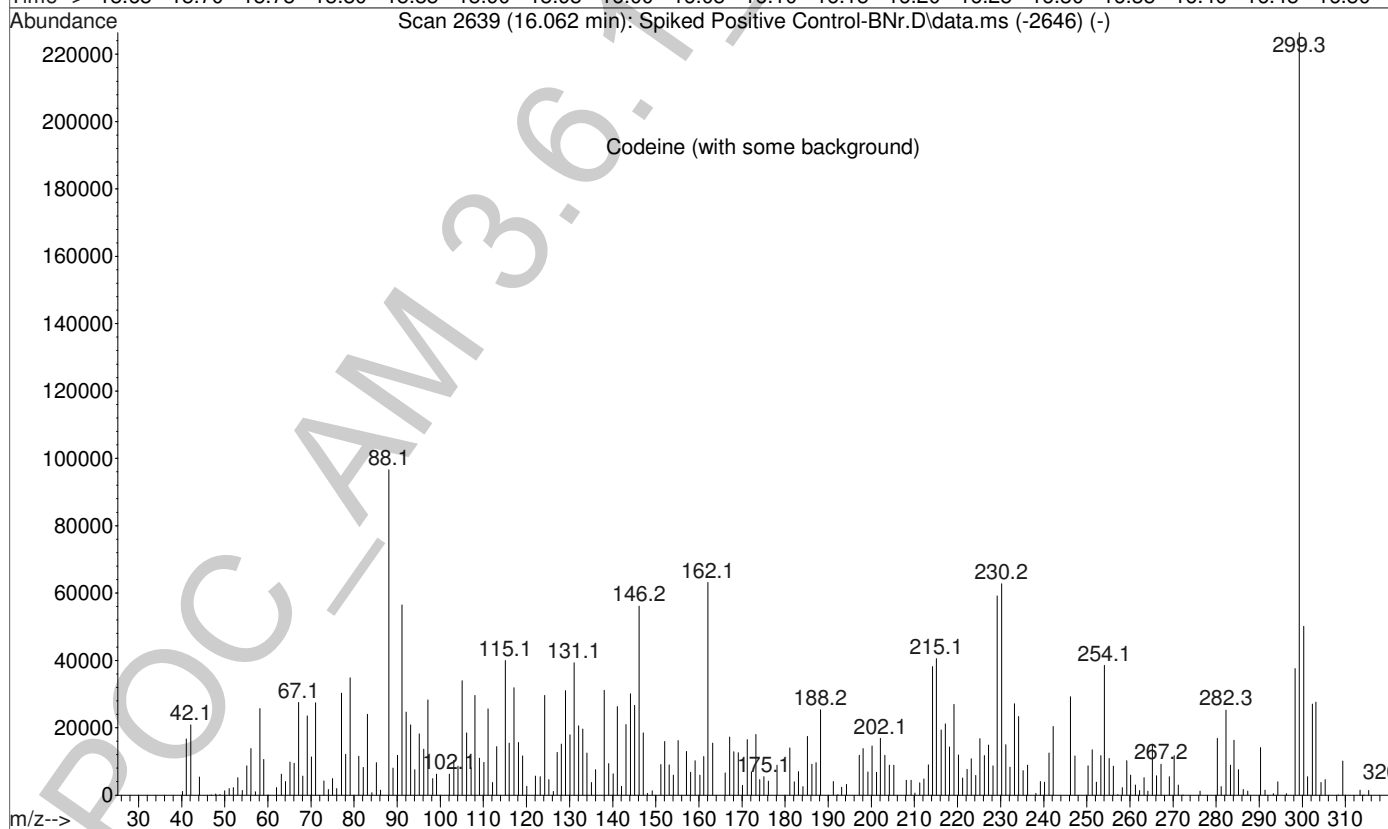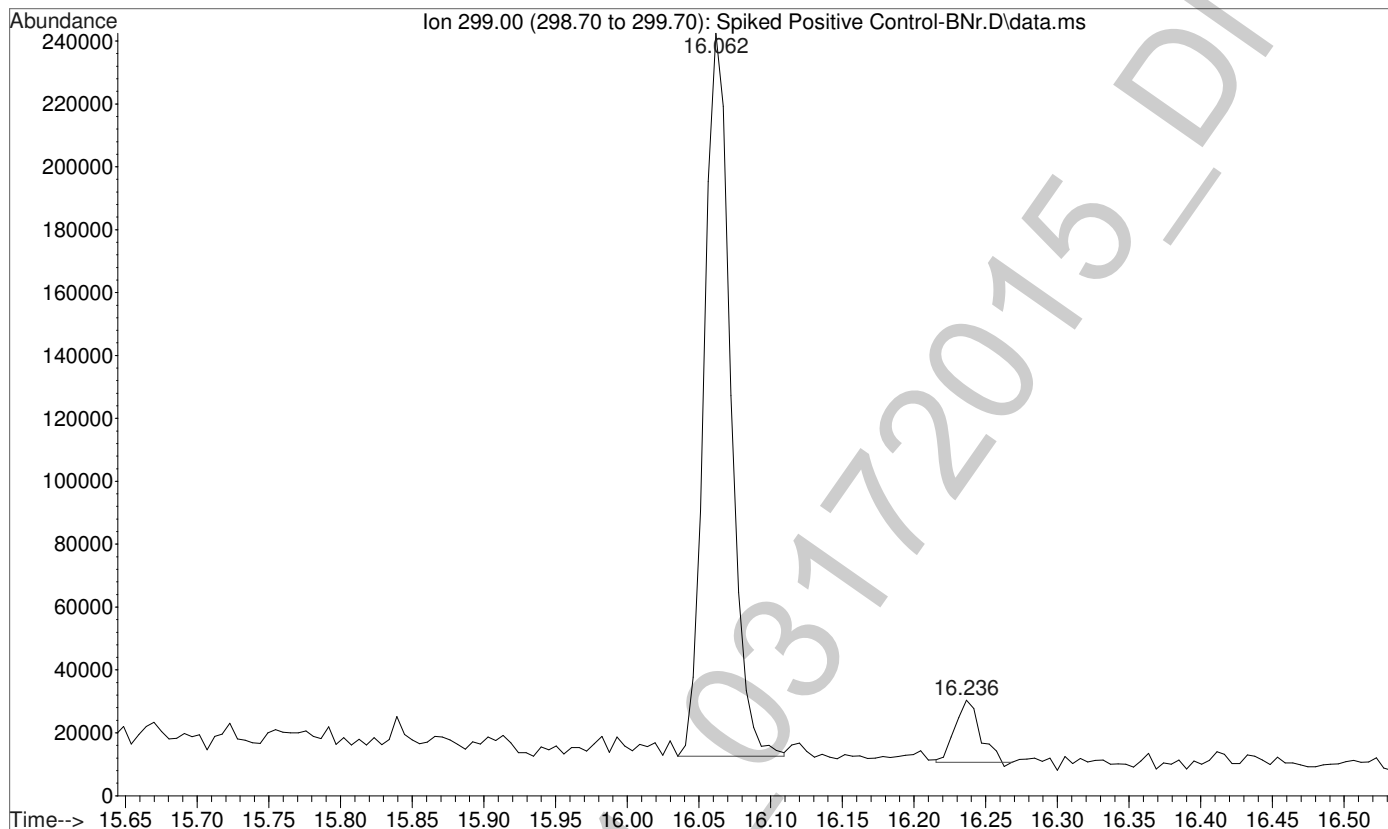



File :C:\gcms\1\data\Blood\031715BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 17 Mar 2015 20:18 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

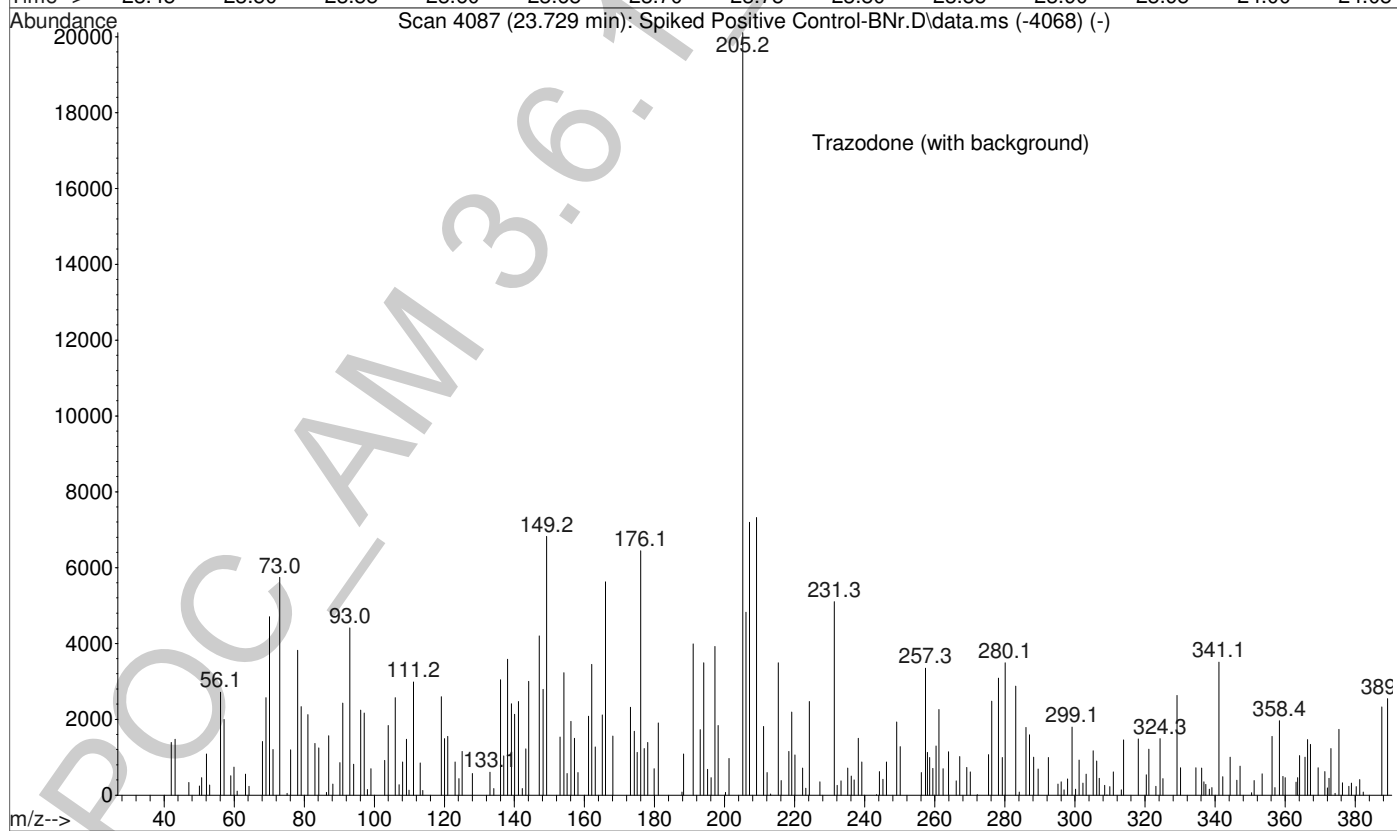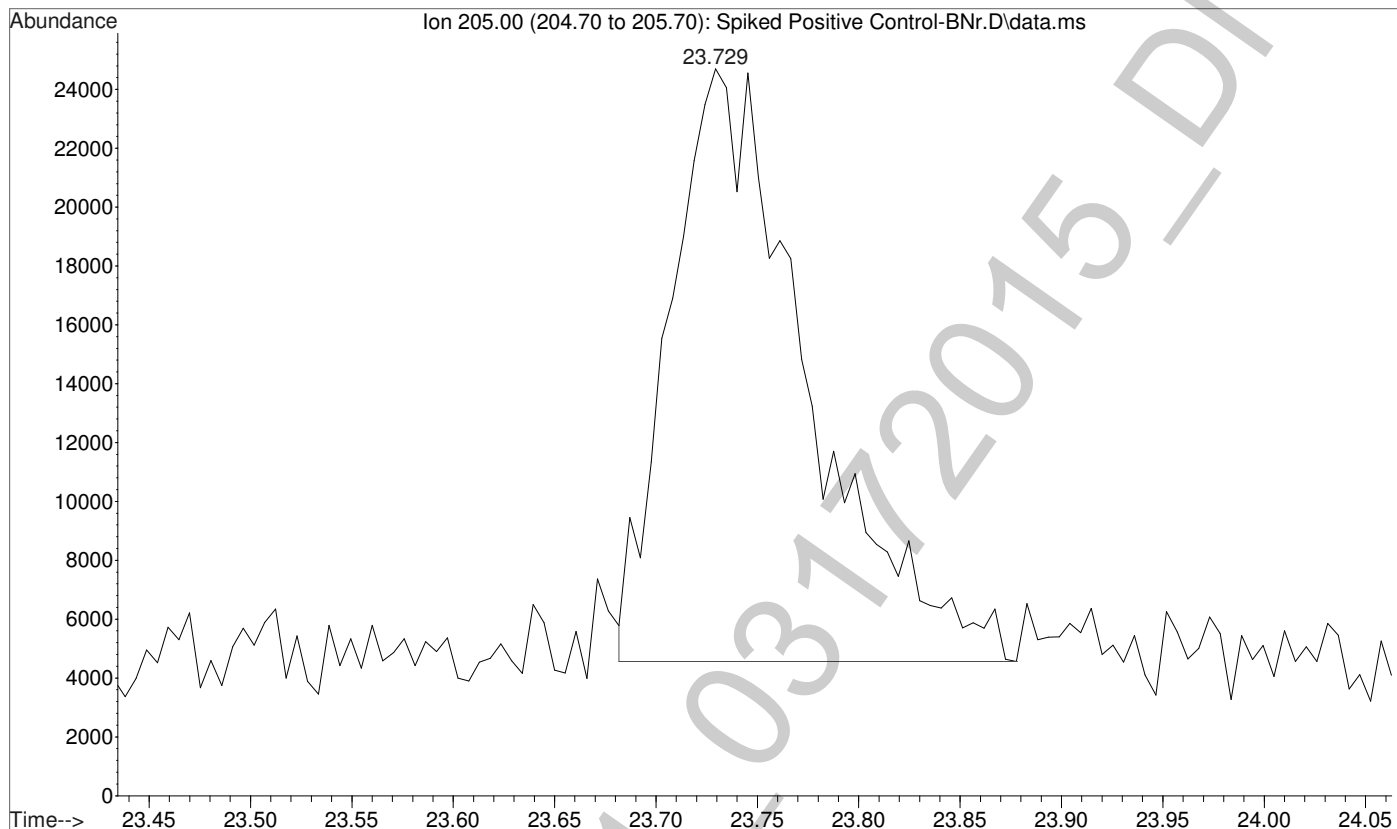

File :C:\gcms\1\data\Blood\031715BN\Reinjection Longer GC Method\p
... rbLK2r.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 17 Mar 2015 20:52 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Solvent Blank
Misc Info : Chloroform

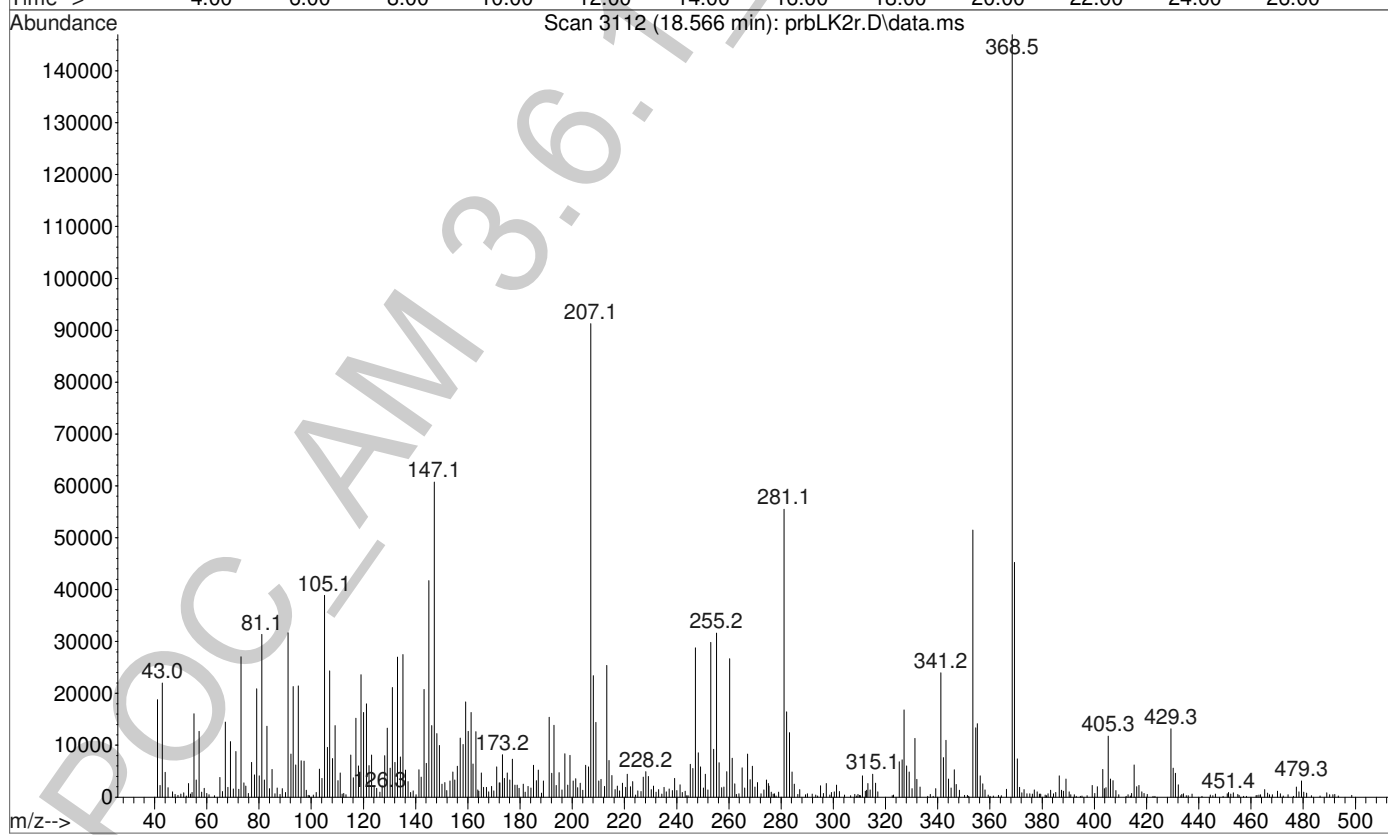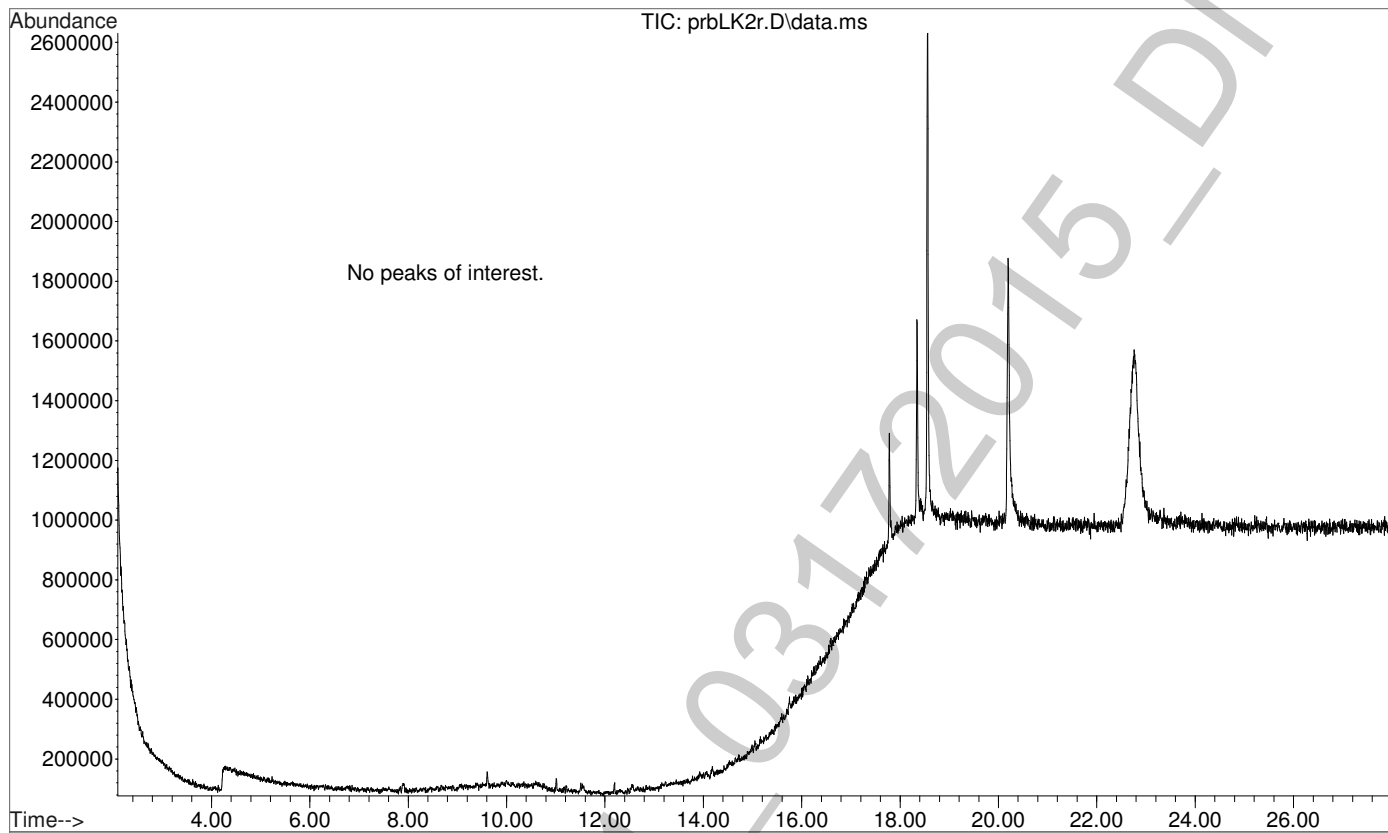

File :C:\gcms\1\data\Blood\031715BN\Reinjection Longer GC Method\P
... OSTBLKr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 19 Mar 2015 19:07 using AcqMethod BNSB120510.M
Sample Name: BLK
Misc Info : Chloroform

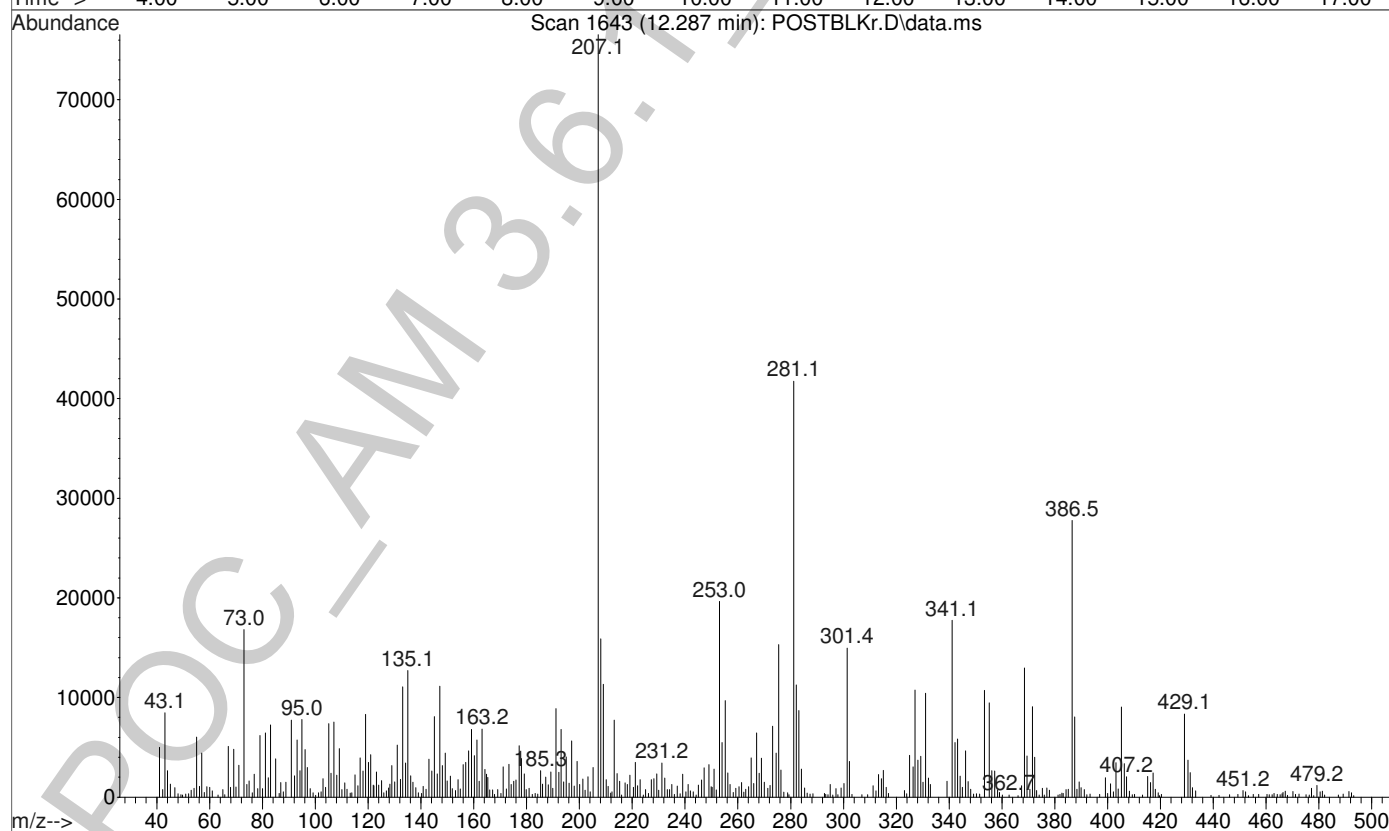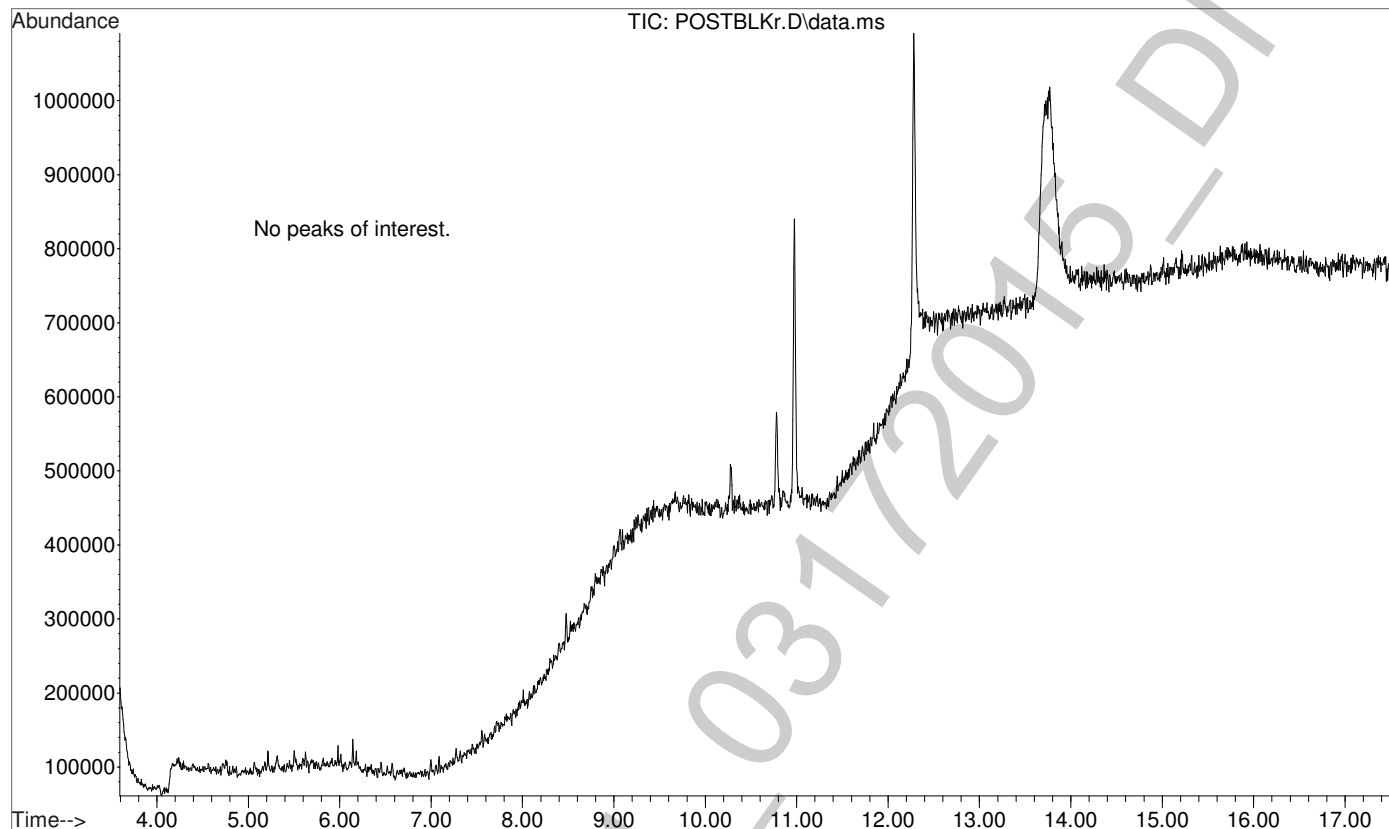

File :C:\gcms\1\data\Blood\031715BN\AFTER.D
Operator : 5LAB-C01\ISPuser
Acquired : 19 Mar 2015 19:29 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: BLK
Misc Info : Chloroform
Vial Number: 73

