


Worklist: 673

<u>LAB_CASE</u>	<u>ITEM</u>	<u>TASK_ID</u>	<u>DESCRIPTION</u>	
C2015-0489	1	30287	3.6.1 Blood base neutral confirr	
C2015-0518	1	30464	3.6.1 Blood base neutral confirr	
C2015-0551	1	30778	3.6.1 Blood base neutral confirr	
C2015-0582	1	31109	3.6.1 Blood base neutral confirr	
M2015-0888	2	32226	3.6.1 Blood base neutral confirr	
M2015-0951	1	30727	3.6.1 Blood base neutral confirr	
M2015-0978	1	32432	3.6.1 Blood base neutral confirr	
M2015-1013	2	31139	3.6.1 Blood base neutral confirr	
M2015-1033	1	32434	3.6.1 Blood base neutral confirr	
M2015-1037	1	31286	3.6.1 Blood base neutral confirr	
M2015-1086	1	31501	3.6.1 Blood base neutral confirr	
M2015-1088	1	31509	3.6.1 Blood base neutral confirr	
M2015-1089	1	31513	3.6.1 Blood base neutral confirr	
M2015-1095	1	31541	3.6.1 Blood base neutral confirr	
M2015-1101	1	31579	3.6.1 Blood base neutral confirr	
M2015-1108	1	31610	3.6.1 Blood base neutral confirr	
M2015-1150	2	31817	3.6.1 Blood base neutral confirr	
P2015-0904	1	31765	3.6.1 Blood base neutral confirr	
P2015-0905	1	31768	3.6.1 Blood base neutral confirr	
P2015-0910	1	31809	3.6.1 Blood base neutral confirr	
P2015-0914	1	31867	3.6.1 Blood base neutral confirr	
P2015-0928	1	31965	3.6.1 Blood base neutral confirr	
P2015-0929	1	31972	3.6.1 Blood base neutral confirr	



Worklist: 673



<u>LAB CASE</u>	<u>ITEM</u>	<u>TASK ID</u>	<u>DESCRIPTION</u>	
P2015-0955	1	32142	3.6.1 Blood base neutral confirr	
P2015-0956	1	32145	3.6.1 Blood base neutral confirr	
P2015-0960	1	32216	3.6.1 Blood base neutral confirr	
P2015-0962	1	32220	3.6.1 Blood base neutral confirr	
P2015-0963	1	32223	3.6.1 Blood base neutral confirr	
P2015-0964	1	32229	3.6.1 Blood base neutral confirr	
P2015-0966	1	32233	3.6.1 Blood base neutral confirr	
P2015-0979	1	32259	3.6.1 Blood base neutral confirr	
P2015-0987	1	32327	3.6.1 Blood base neutral confirr	
P2015-1010	1	32415	3.6.1 Blood base neutral confirr	

POC_AM 3.6.1_042125

04/21/15

simulate_sequence.log
Simulate Run Sequence Tue Apr 21 11:17:10 2015

Instrument Name: Major Mass Spec
Sequence File: C:\Users\ISPuser\Desktop\Sequences\DD-BNSB.sequence.xml
Comment: MassHunter sequence
Operator: 5LAB-C01\ISPuser
Data Path: D:\DATA\DND\2015\042115BN\
Method Path: D:\MassHunter\GCMS\1\methods\

Line	Type	Vials	DataFile	Sample Name
Acquisition Method: BNSB120510.M				
1)	Sample	100	Prerun Solvent Blank	Pre-run Solvent Blank
2)	Sample	1	Negative Control-BN	Negative Control -
...0689				
3)	Sample	2	Spiked Positive Control-BN	Positive Control
4)	Sample	99	prbLK2	Solvent Blank
Acquisition Method: GBT092509-Delta EMV.M				
5)	Sample	100	Prerun Solvent Blankr	Pre-run Solvent Blank
6)	Sample	1	Negative Control-BNr	Negative Control -
...0689				
7)	Sample	2	Spiked Positive Control-BNr	Positive Control
8)	Sample	99	prbLK2r	Solvent Blank
Acquisition Method: BNSB120510.M				
9)	Sample	98	C2015-0489-1-BNBLK	Lab No.: C2015-0489-1
10)	Sample	3	C2015-0489-1-BN	Lab No.: C2015-0489-1
11)	Sample	97	C2015-0518-1-BNBLK	Lab No.: C2015-0518-1
12)	Sample	4	C2015-0518-1-BN	Lab No.: C2015-0518-1
13)	Sample	96	C2015-0551-1-BNBLK	Lab No.: C2015-0551-1
14)	Sample	5	C2015-0551-1-BN	Lab No.: C2015-0551-1
15)	Sample	95	C2015-0582-1-BNBLK	Lab No.: C2015-0582-1
16)	Sample	6	C2015-0582-1-BN	Lab No.: C2015-0582-1
17)	Sample	94	M2015-0888-2-BNBLK	Lab No.: M2015-0888-2
18)	Sample	7	M2015-0888-2-BN	Lab No.: M2015-0888-2
19)	Sample	93	M2015-0951-1-BNBLK	Lab No.: M2015-0951-1
20)	Sample	8	M2015-0951-1-BN	Lab No.: M2015-0951-1
21)	Sample	92	M2015-0978-1-BNBLK	Lab No.: M2015-0978-1
22)	Sample	9	M2015-0978-1-BN	Lab No.: M2015-0978-1
23)	Sample	91	M2015-1013-2-BNBLK	Lab No.: M2015-1013-2
24)	Sample	10	M2015-1013-2-BN	Lab No.: M2015-1013-2
Acquisition Method: GBT092509-Delta EMV.M				
25)	Sample	98	C2015-0489-1-BNBLKr	Lab No.: C2015-0489-1
26)	Sample	3	C2015-0489-1-BNr	Lab No.: C2015-0489-1
27)	Sample	97	C2015-0518-1-BNBLKr	Lab No.: C2015-0518-1
28)	Sample	4	C2015-0518-1-BNr	Lab No.: C2015-0518-1
29)	Sample	96	C2015-0551-1-BNBLKr	Lab No.: C2015-0551-1
30)	Sample	5	C2015-0551-1-BNr	Lab No.: C2015-0551-1
31)	Sample	95	C2015-0582-1-BNBLKr	Lab No.: C2015-0582-1
32)	Sample	6	C2015-0582-1-BNr	Lab No.: C2015-0582-1
33)	Sample	94	M2015-0888-2-BNBLKr	Lab No.: M2015-0888-2
34)	Sample	7	M2015-0888-2-BNr	Lab No.: M2015-0888-2
35)	Sample	93	M2015-0951-1-BNBLKr	Lab No.: M2015-0951-1
36)	Sample	8	M2015-0951-1-BNr	Lab No.: M2015-0951-1
37)	Sample	92	M2015-0978-1-BNBLKr	Lab No.: M2015-0978-1
38)	Sample	9	M2015-0978-1-BNr	Lab No.: M2015-0978-1
39)	Sample	91	M2015-1013-2-BNBLKr	Lab No.: M2015-1013-2
40)	Sample	10	M2015-1013-2-BNr	Lab No.: M2015-1013-2
Acquisition Method: BNSB120510.M				
41)	Sample	90	M2015-1033-1-BNBLK	Lab No.: M2015-1033-1
42)	Sample	11	M2015-1033-1-BN	Lab No.: M2015-1033-1
43)	Sample	89	M2015-1037-1-BNBLK	Lab No.: M2015-1037-1
44)	Sample	12	M2015-1037-1-BN	Lab No.: M2015-1037-1

04/21/15.

simulate_sequence.log
45) Sample 88 ✓ M2015-1086-1-BNBLK Lab No.: M2015-1086-1
46) Sample 13 ✓ M2015-1086-1-BN Lab No.: M2015-1086-1
47) Sample 87 ✓ M2015-1088-1-BNBLK Lab No.: M2015-1088-1
48) Sample 14 ✓ M2015-1088-1-BN Lab No.: M2015-1088-1
49) Sample 86 ✓ M2015-1089-1-BNBLK Lab No.: M2015-1089-1
50) Sample 15 ✓ M2015-1089-1-BN Lab No.: M2015-1089-1

Acquisition Method: GBT092509-Delta EMV.M
51) Sample 90 ✓ M2015-1033-1-BNBLKr Lab No.: M2015-1033-1
52) Sample 11 ✓ M2015-1033-1-BNr Lab No.: M2015-1033-1
53) Sample 89 ✓ M2015-1037-1-BNBLKr Lab No.: M2015-1037-1
54) Sample 12 ✓ M2015-1037-1-BNr Lab No.: M2015-1037-1
55) Sample 88 ✓ M2015-1086-1-BNBLKr Lab No.: M2015-1086-1
56) Sample 13 ✓ M2015-1086-1-BNr Lab No.: M2015-1086-1
57) Sample 87 ✓ M2015-1088-1-BNBLKr Lab No.: M2015-1088-1
58) Sample 14 ✓ M2015-1088-1-BNr Lab No.: M2015-1088-1
59) Sample 86 ✓ M2015-1089-1-BNBLKr Lab No.: M2015-1089-1
60) Sample 15 ✓ M2015-1089-1-BNr Lab No.: M2015-1089-1

Acquisition Method: BNSB120510.M
61) Sample 85 ✓ M2015-1095-1-BNBLK Lab No.: M2015-1095-1
62) Sample 16 ✓ M2015-1095-1-BN Lab No.: M2015-1095-1
63) Sample 84 ✓ M2015-1101-1-BNBLK Lab No.: M2015-1101-1
64) Sample 17 ✓ M2015-1101-1-BN Lab No.: M2015-1101-1
65) Sample 83 ✓ M2015-1108-1-BNBLK Lab No.: M2015-1108-1
66) Sample 18 ✓ M2015-1108-1-BN Lab No.: M2015-1108-1
67) Sample 82 ✓ M2015-1150-2-BNBLK Lab No.: M2015-1150-2
68) Sample 19 ✓ M2015-1150-2-BN Lab No.: M2015-1150-2
69) Sample 81 ✓ P2015-0904-1-BNBLK Lab No.: P2015-0904-1
70) Sample 20 ✓ P2015-0904-1-BN Lab No.: P2015-0904-1

Acquisition Method: GBT092509-Delta EMV.M
71) Sample 85 ✓ M2015-1095-1-BNBLKr Lab No.: M2015-1095-1
72) Sample 16 ✓ M2015-1095-1-BNr Lab No.: M2015-1095-1
73) Sample 84 ✓ M2015-1101-1-BNBLKr Lab No.: M2015-1101-1
74) Sample 17 ✓ M2015-1101-1-BNr Lab No.: M2015-1101-1
75) Sample 83 ✓ M2015-1108-1-BNBLKr Lab No.: M2015-1108-1
76) Sample 18 ✓ M2015-1108-1-BNr Lab No.: M2015-1108-1
77) Sample 82 ✓ M2015-1150-2-BNBLKr Lab No.: M2015-1150-2
78) Sample 19 ✓ M2015-1150-2-BNr Lab No.: M2015-1150-2
79) Sample 81 ✓ P2015-0904-1-BNBLKr Lab No.: P2015-0904-1
80) Sample 20 ✓ P2015-0904-1-BNr Lab No.: P2015-0904-1

Acquisition Method: BNSB120510.M
81) Sample 80 ✓ P2015-0905-1-BNBLK Lab No.: P2015-0905-1
82) Sample 21 ✓ P2015-0905-1-BN Lab No.: P2015-0905-1
83) Sample 79 ✓ P2015-0910-1-BNBLK Lab No.: P2015-0910-1
84) Sample 22 ✓ P2015-0910-1-BN Lab No.: P2015-0910-1
85) Sample 78 ✓ P2015-0914-1-BNBLK Lab No.: P2015-0914-1
86) Sample 23 ✓ P2015-0914-1-BN Lab No.: P2015-0914-1
87) Sample 77 ✓ P2015-0928-1-BNBLK Lab No.: P2015-0928-1
88) Sample 24 ✓ P2015-0928-1-BN Lab No.: P2015-0928-1
89) Sample 76 ✓ P2015-0929-1-BNBLK Lab No.: P2015-0929-1
90) Sample 25 ✓ P2015-0929-1-BN Lab No.: P2015-0929-1

Acquisition Method: GBT092509-Delta EMV.M
91) Sample 80 ✓ P2015-0905-1-BNBLKr Lab No.: P2015-0905-1
92) Sample 21 ✓ P2015-0905-1-BNr Lab No.: P2015-0905-1
93) Sample 79 ✓ P2015-0910-1-BNBLKr Lab No.: P2015-0910-1
94) Sample 22 ✓ P2015-0910-1-BNr Lab No.: P2015-0910-1
95) Sample 78 ✓ P2015-0914-1-BNBLKr Lab No.: P2015-0914-1
96) Sample 23 ✓ P2015-0914-1-BNr Lab No.: P2015-0914-1
97) Sample 77 ✓ P2015-0928-1-BNBLKr Lab No.: P2015-0928-1
98) Sample 24 ✓ P2015-0928-1-BNr Lab No.: P2015-0928-1
99) Sample 76 ✓ P2015-0929-1-BNBLKr Lab No.: P2015-0929-1
100) Sample 25 ✓ P2015-0929-1-BNr Lab No.: P2015-0929-1

Acquisition Method: BNSB120510.M

04/21/15

simulate_sequence.log
101) Sample 75 ✓ P2015-0955-1-BNBLK Lab No.: P2015-0955-1
102) Sample 26 ✓ P2015-0955-1-BN Lab No.: P2015-0955-1
103) Sample 74 ✓ P2015-0956-1-BNBLK Lab No.: P2015-0956-1
104) Sample 27 ✓ P2015-0956-1-BN Lab No.: P2015-0956-1
105) Sample 73 ✓ P2015-0960-1-BNBLK Lab No.: P2015-0960-1
106) Sample 28 ✓ P2015-0960-1-BN Lab No.: P2015-0960-1
107) Sample 72 ✓ P2015-0962-1-BNBLK Lab No.: P2015-0962-1
108) Sample 29 ✓ P2015-0962-1-BN Lab No.: P2015-0962-1
109) Sample 71 ✓ P2015-0963-1-BNBLK Lab No.: P2015-0963-1
110) Sample 30 ✓ P2015-0963-1-BN Lab No.: P2015-0963-1

Acquisition Method: GBT092509-Delta EMV.M
111) Sample 75 ✓ P2015-0955-1-BNBLKr Lab No.: P2015-0955-1
112) Sample 26 ✓ P2015-0955-1-BNr Lab No.: P2015-0955-1
113) Sample 74 ✓ P2015-0956-1-BNBLKr Lab No.: P2015-0956-1
114) Sample 27 ✓ P2015-0956-1-BNr Lab No.: P2015-0956-1
115) Sample 73 ✓ P2015-0960-1-BNBLKr Lab No.: P2015-0960-1
116) Sample 28 ✓ P2015-0960-1-BNr Lab No.: P2015-0960-1
117) Sample 72 ✓ P2015-0962-1-BNBLKr Lab No.: P2015-0962-1
118) Sample 29 ✓ P2015-0962-1-BNr Lab No.: P2015-0962-1
119) Sample 71 ✓ P2015-0963-1-BNBLKr Lab No.: P2015-0963-1
120) Sample 30 ✓ P2015-0963-1-BNr Lab No.: P2015-0963-1

Acquisition Method: BNSB120510.M
121) Sample 70 ✓ P2015-0964-1-BNBLK Lab No.: P2015-0964-1
122) Sample 31 ✓ P2015-0964-1-BN Lab No.: P2015-0964-1
123) Sample 69 ✓ P2015-0966-1-BNBLK Lab No.: P2015-0966-1
124) Sample 32 ✓ P2015-0966-1-BN Lab No.: P2015-0966-1
125) Sample 68 ✓ P2015-0979-1-BNBLK Lab No.: P2015-0979-1
126) Sample 33 ✓ P2015-0979-1-BN Lab No.: P2015-0979-1
127) Sample 67 ✓ P2015-0987-1-BNBLK Lab No.: P2015-0987-1
128) Sample 34 ✓ P2015-0987-1-BN Lab No.: P2015-0987-1
129) Sample 66 ✓ P2015-1010-1-BNBLK Lab No.: P2015-1010-1
130) Sample 35 ✓ P2015-1010-1-BN Lab No.: P2015-1010-1

Acquisition Method: GBT092509-Delta EMV.M
131) Sample 70 ✓ P2015-0964-1-BNBLKr Lab No.: P2015-0964-1
132) Sample 31 ✓ P2015-0964-1-BNr Lab No.: P2015-0964-1
133) Sample 69 ✓ P2015-0966-1-BNBLKr Lab No.: P2015-0966-1
134) Sample 32 ✓ P2015-0966-1-BNr Lab No.: P2015-0966-1
135) Sample 68 ✓ P2015-0979-1-BNBLKr Lab No.: P2015-0979-1
136) Sample 33 ✓ P2015-0979-1-BNr Lab No.: P2015-0979-1
137) Sample 67 ✓ P2015-0987-1-BNBLKr Lab No.: P2015-0987-1
138) Sample 34 ✓ P2015-0987-1-BNr Lab No.: P2015-0987-1
139) Sample 66 ✓ P2015-1010-1-BNBLKr Lab No.: P2015-1010-1
140) Sample 35 ✓ P2015-1010-1-BNr Lab No.: P2015-1010-1

Acquisition Method: BNSB120510.M
141) Sample 65 ✓ POSTBLKr BLK

Acquisition Method: GBT092509-Delta EMV.M
142) Sample 64 ✓ AFTER BLK
megabytes Needed: 3589 Space on drive D: 299941
Sequence Verification Done!

POC-IM3

Analytical Method 3.6.1 & 3.6.7 QA Check List

Run Start Date: 04/21/15

Analyst: DND

(Short GC/MS temperature program)



Positive Control Compound List



- Methamphetamine
- Nicotine
- Meperidine
- Caffeine
- Diphenhydramine
- Lidocaine
- PCP
- Methadone
- Amitriptyline
- Codeine
- Trazodone

Internal Standards


- Benzphetamine
- Papaverine

Optional back extraction **not** performed.
Samples reconstituted in methanol.



File :C:\gcms\1\data\Blood\042115BN\Prerun Solvent Blank.D
Operator : 5LAB-C01\ISPuser
Acquired : 21 Apr 2015 11:21 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Pre-run Solvent Blank
Misc Info : Chloroform
Vial Number: 100

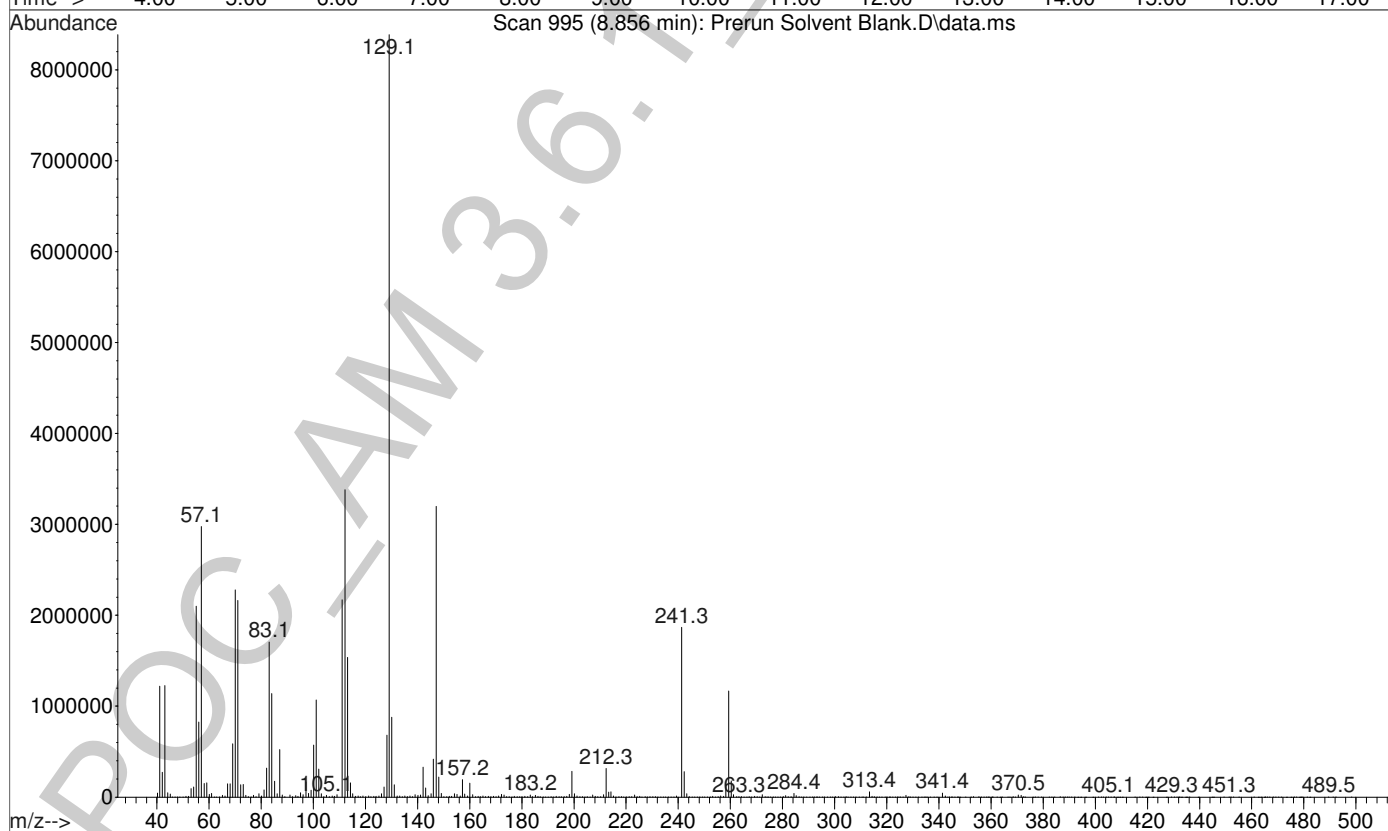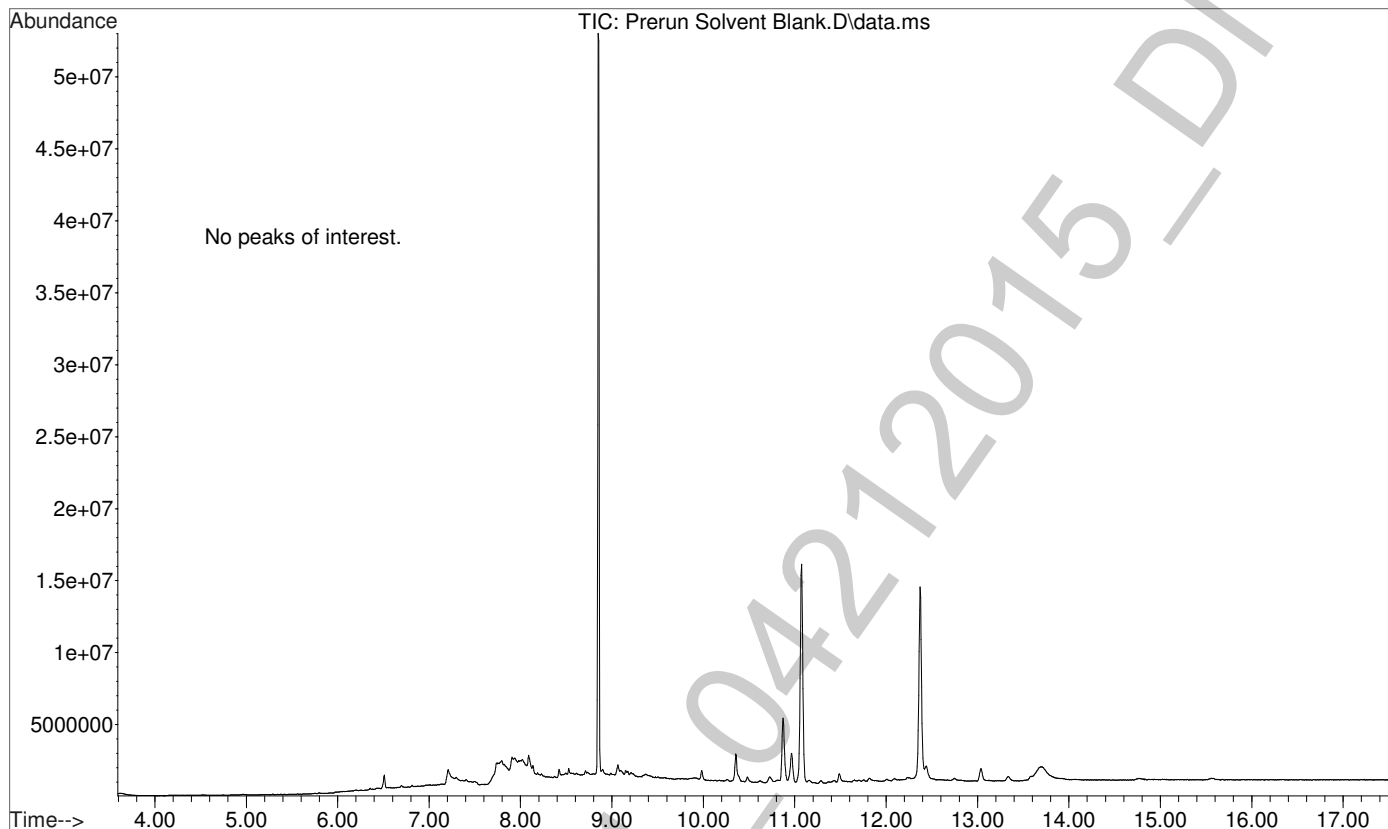



File :C:\gcms\1\data\Blood\042115BN\Negative Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 21 Apr 2015 11:44 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1
Vial Number: 1

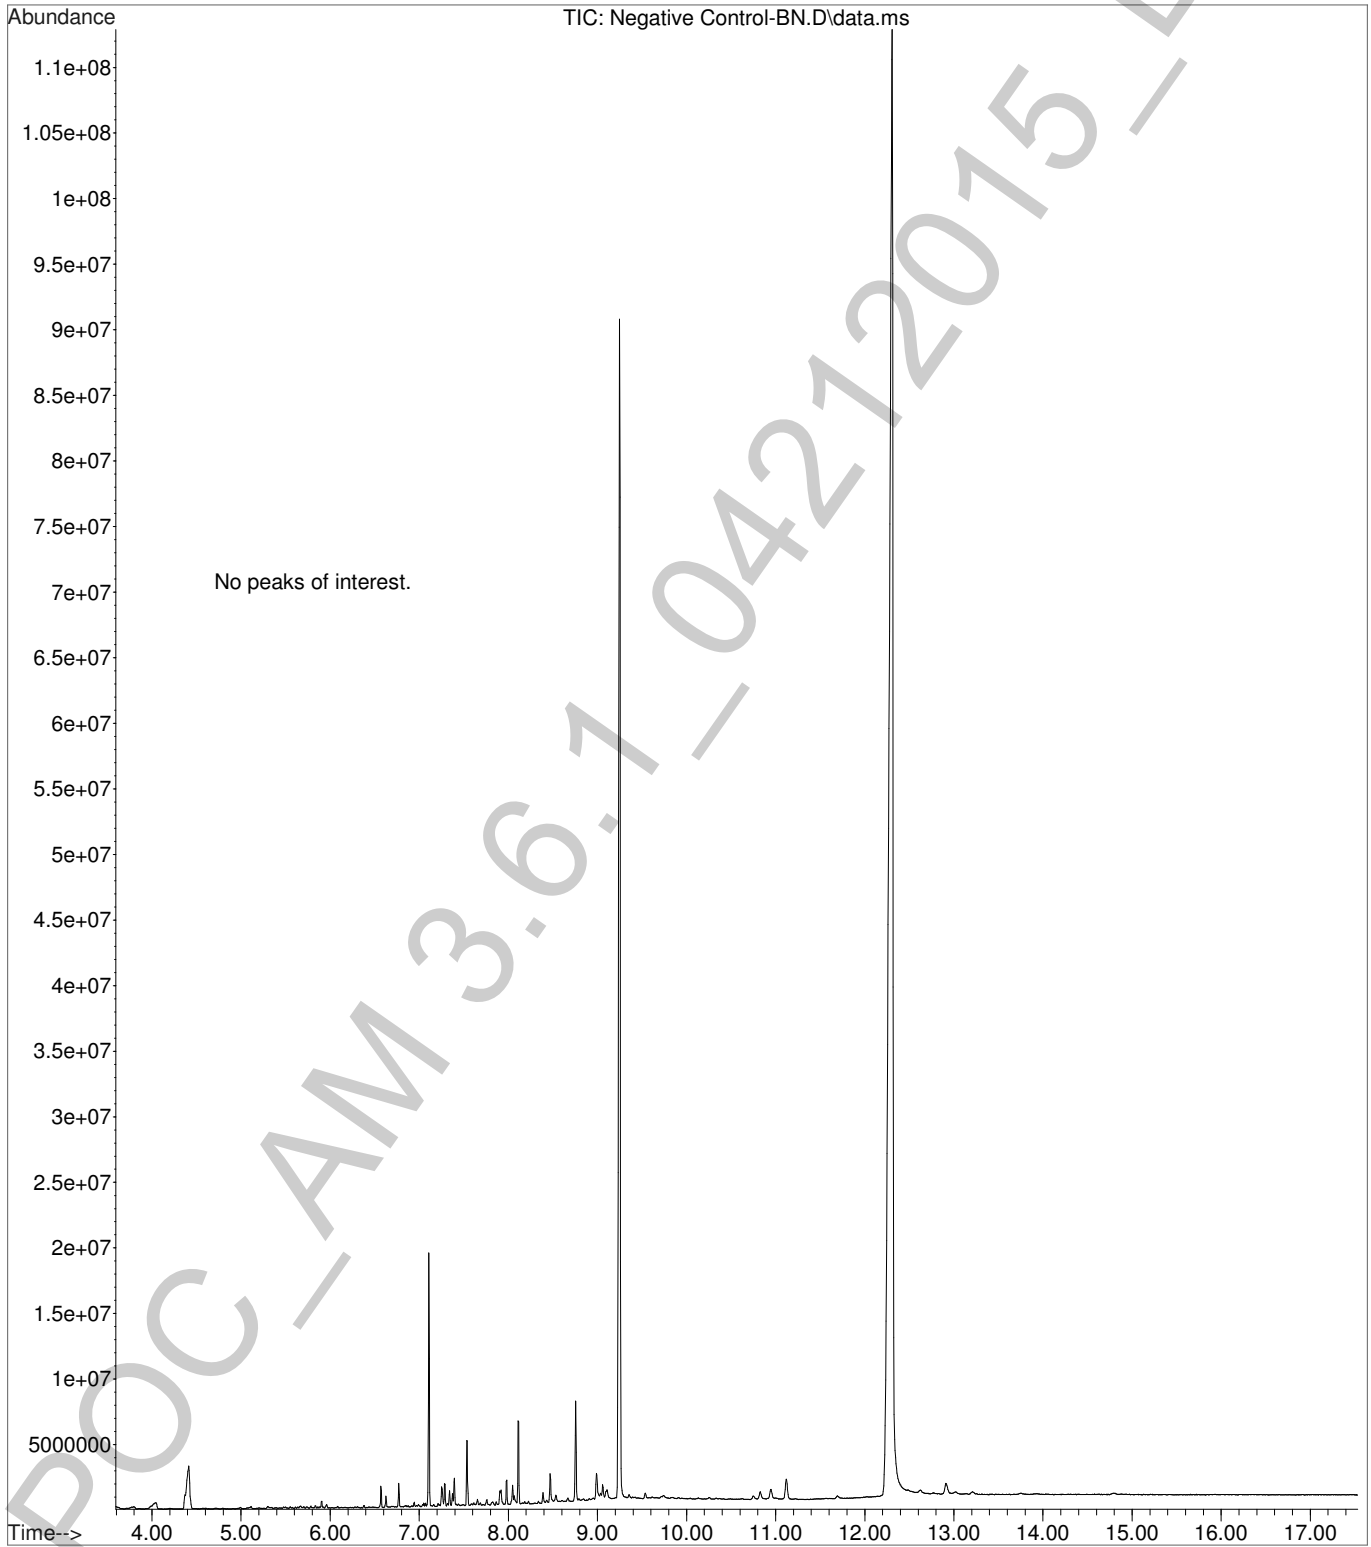


File :C:\gcms\1\data\Blood\042115BN\Negative Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 21 Apr 2015 11:44 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1
Vial Number: 1

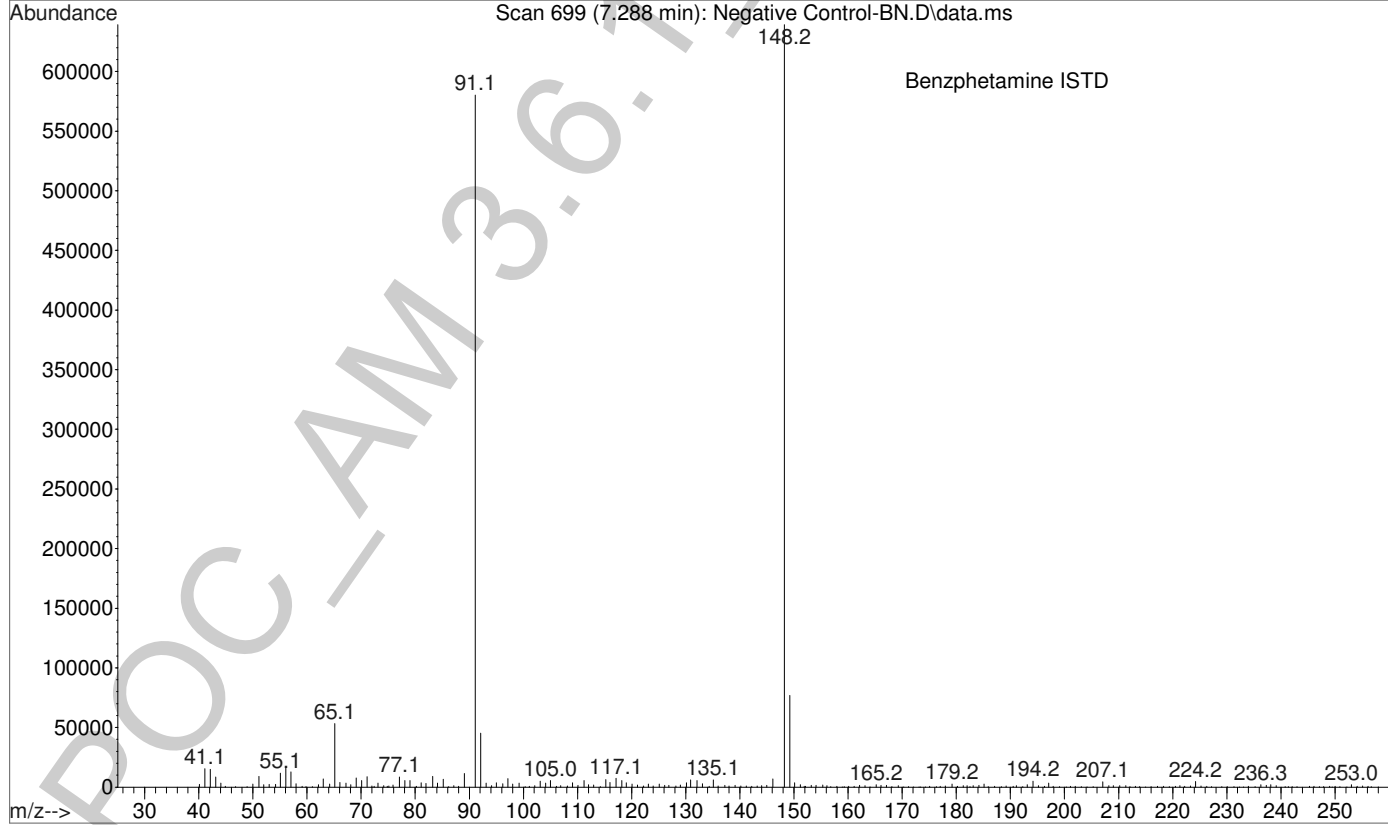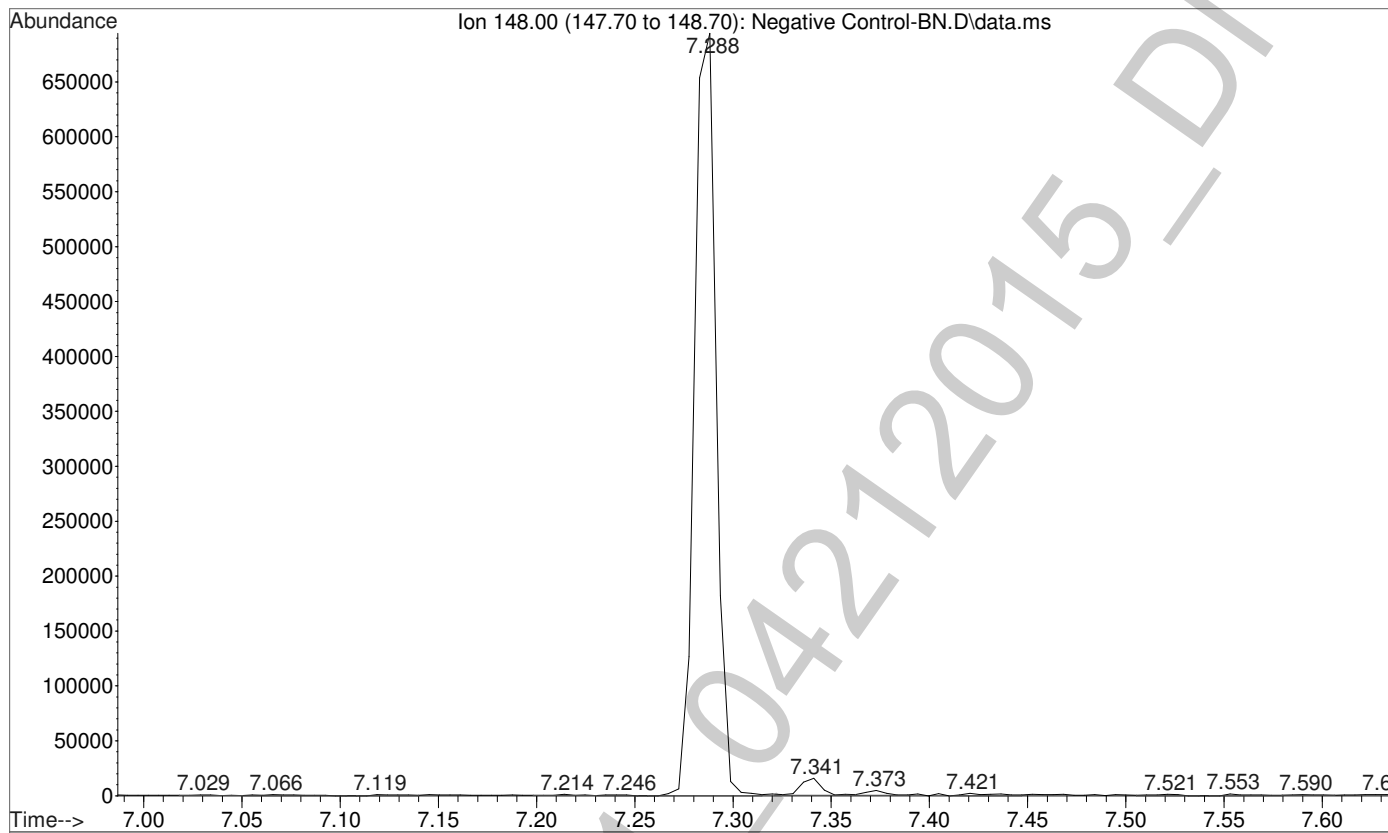



File :C:\gcms\1\data\Blood\042115BN\Negative Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 21 Apr 2015 11:44 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1
Vial Number: 1

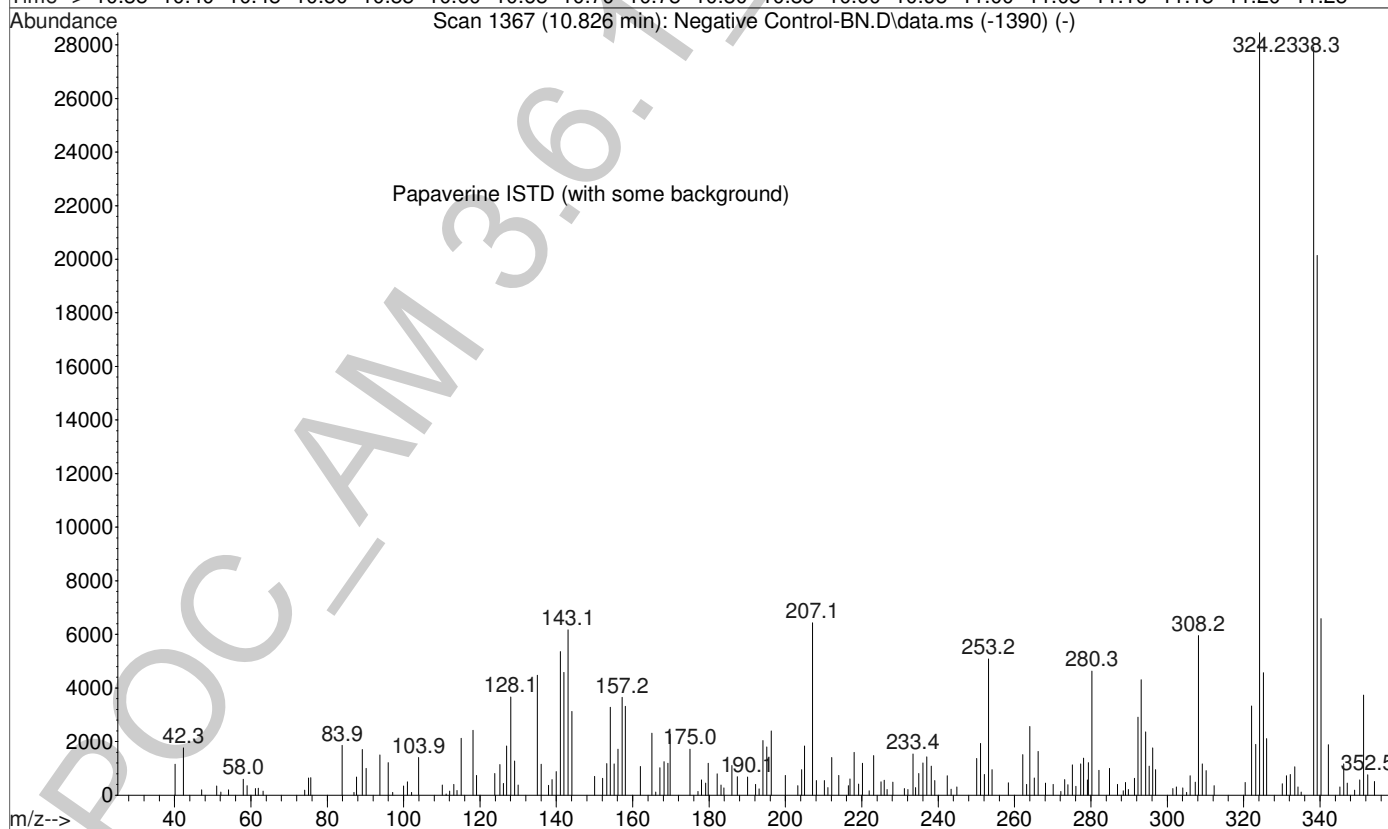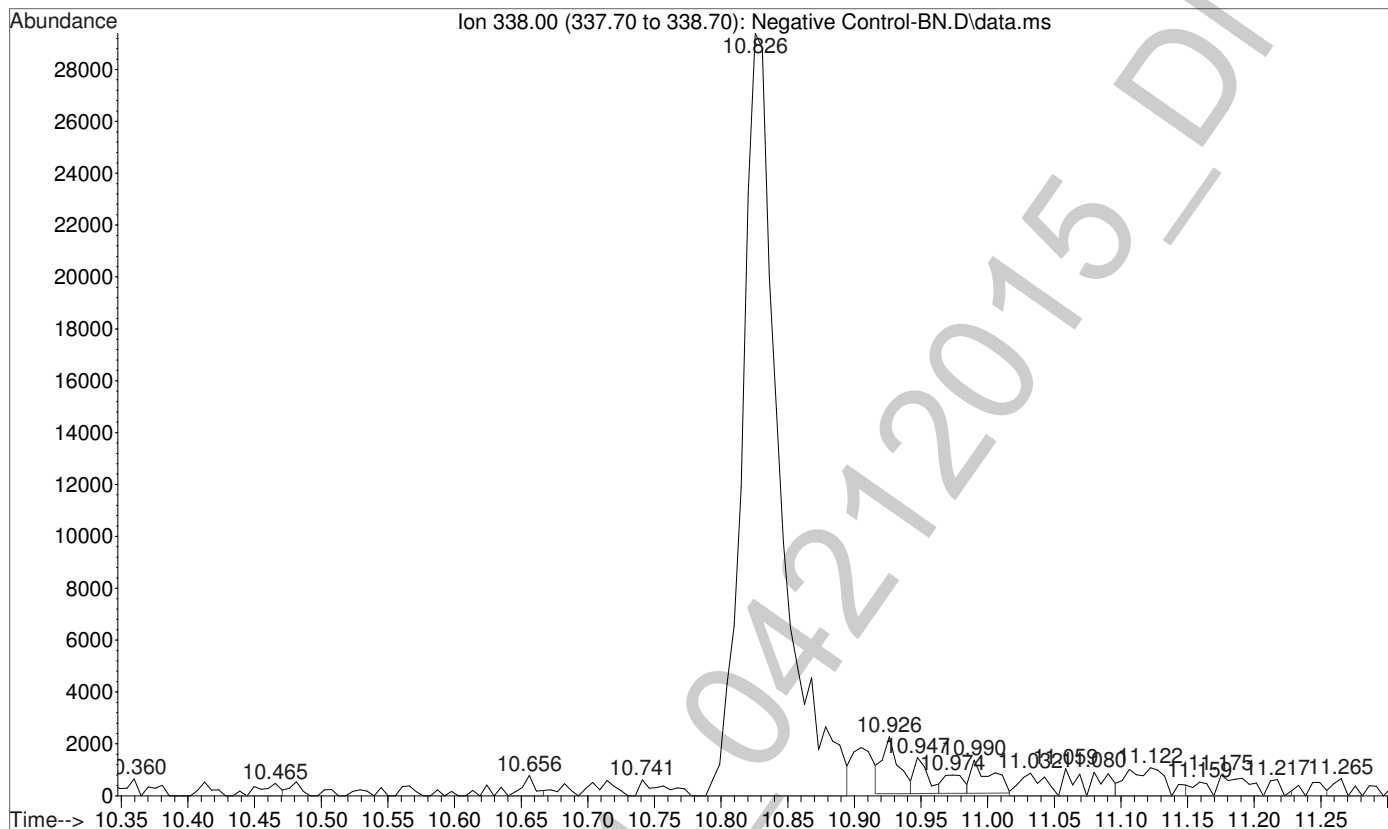



File :C:\gcms\1\data\Blood\042115BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 21 Apr 2015 12:07 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

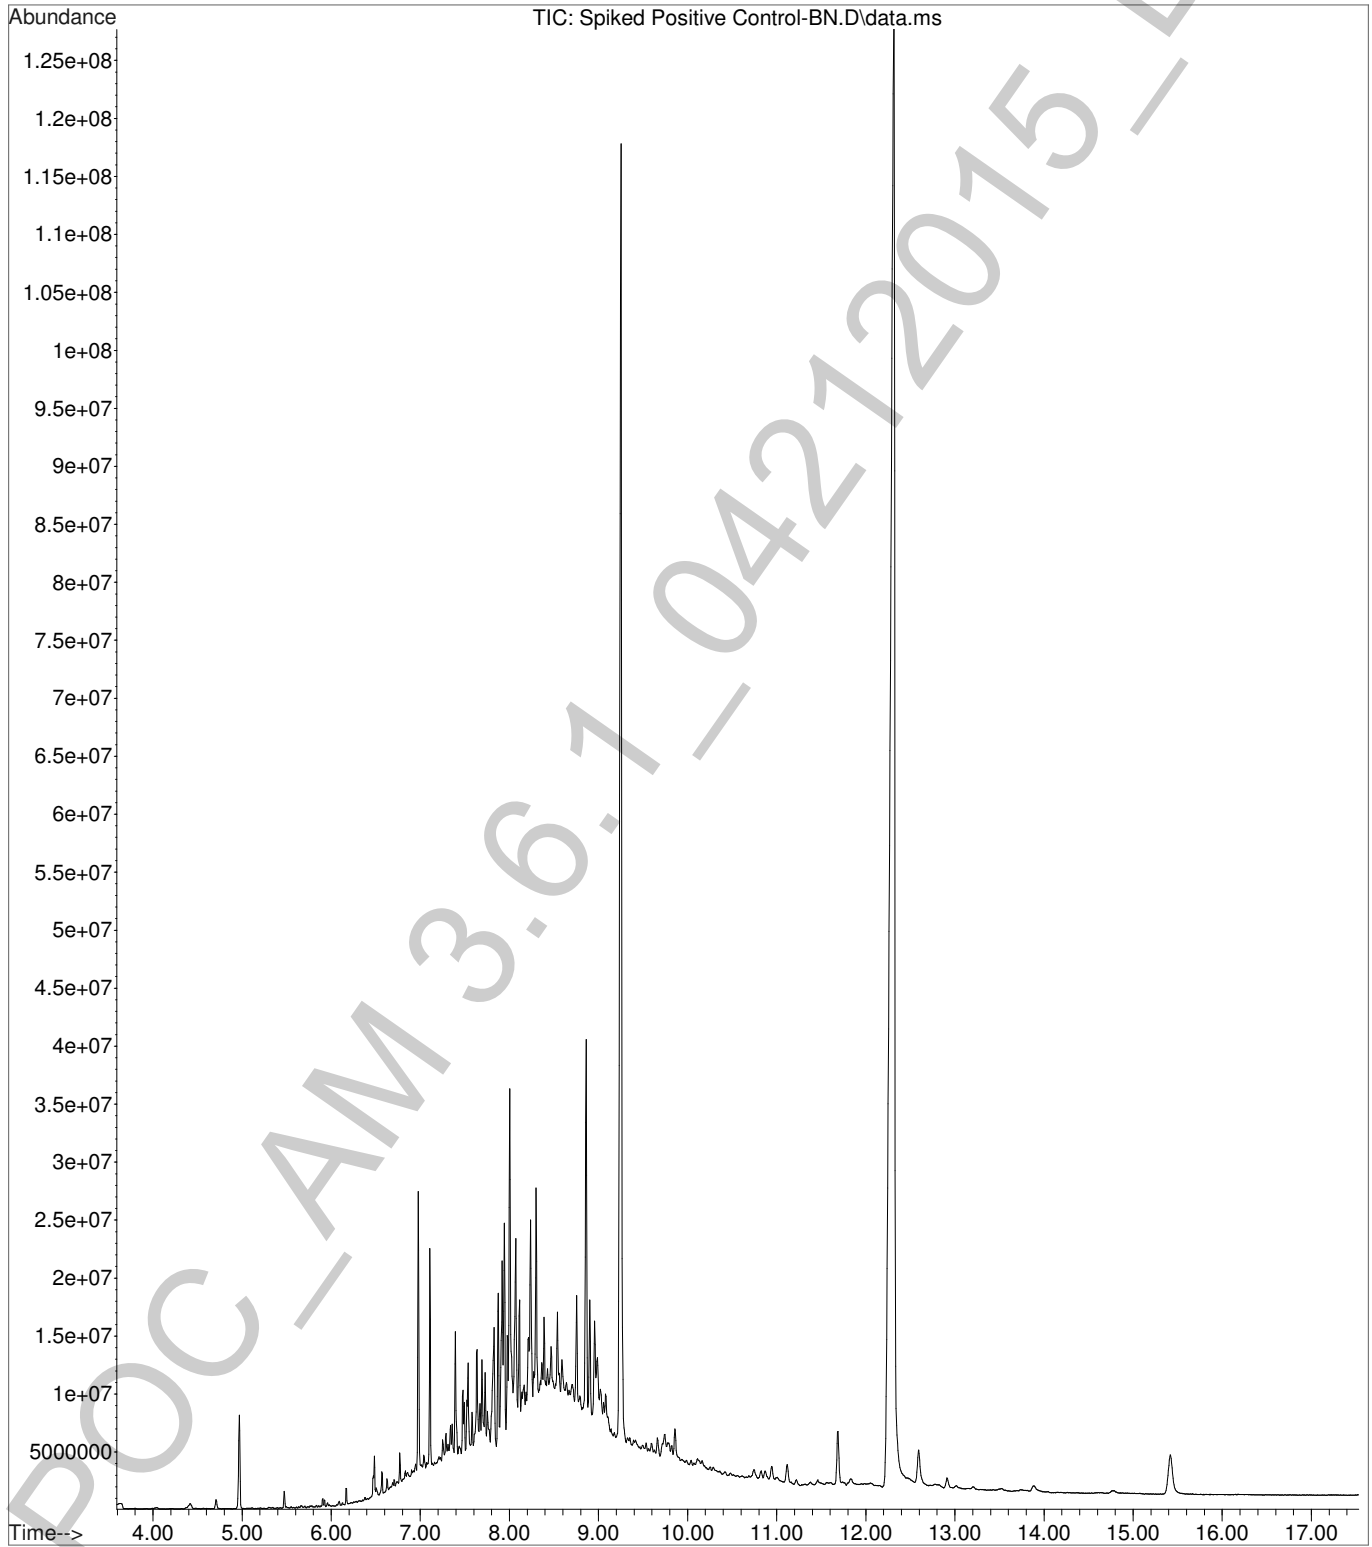



File :C:\gcms\1\data\Blood\042115BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 21 Apr 2015 12:07 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

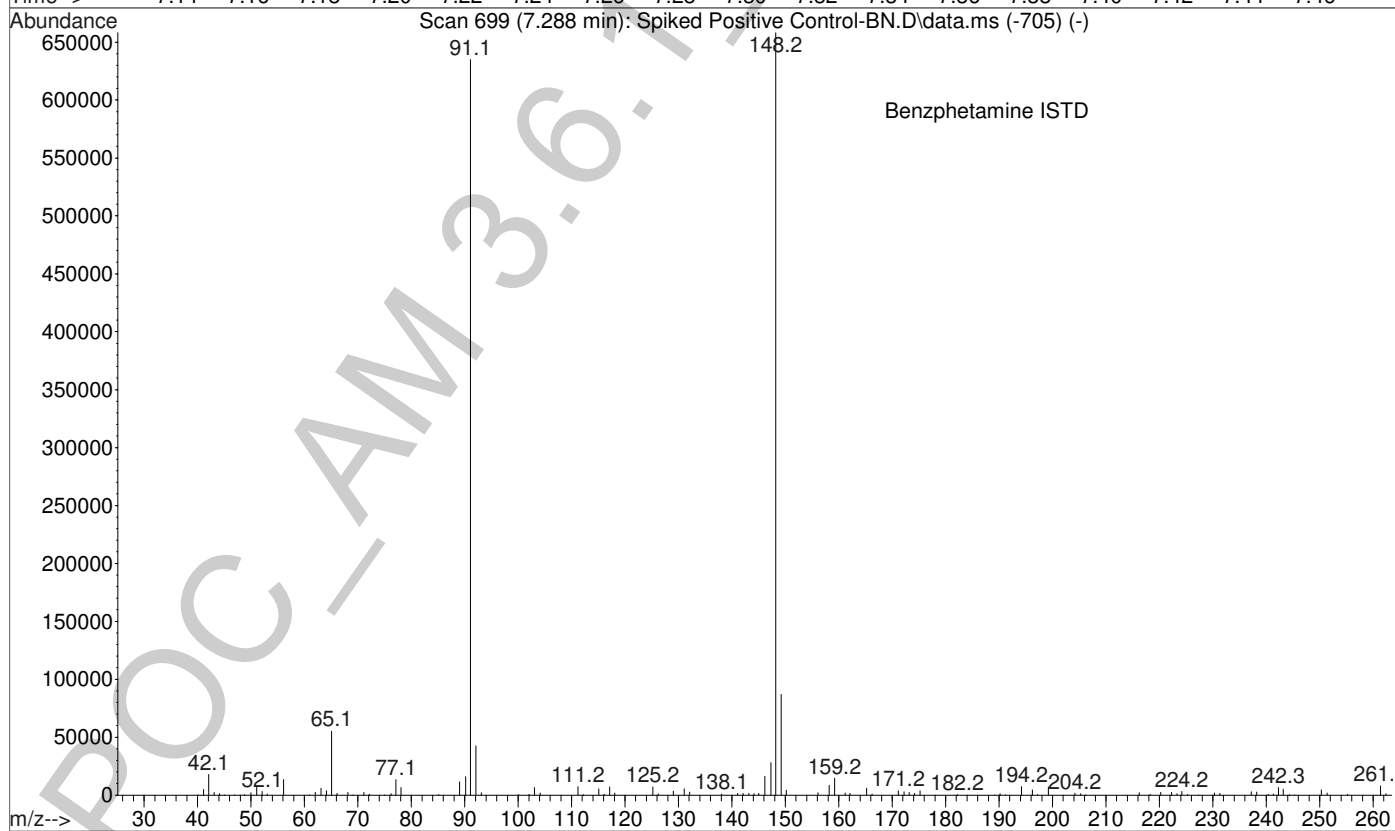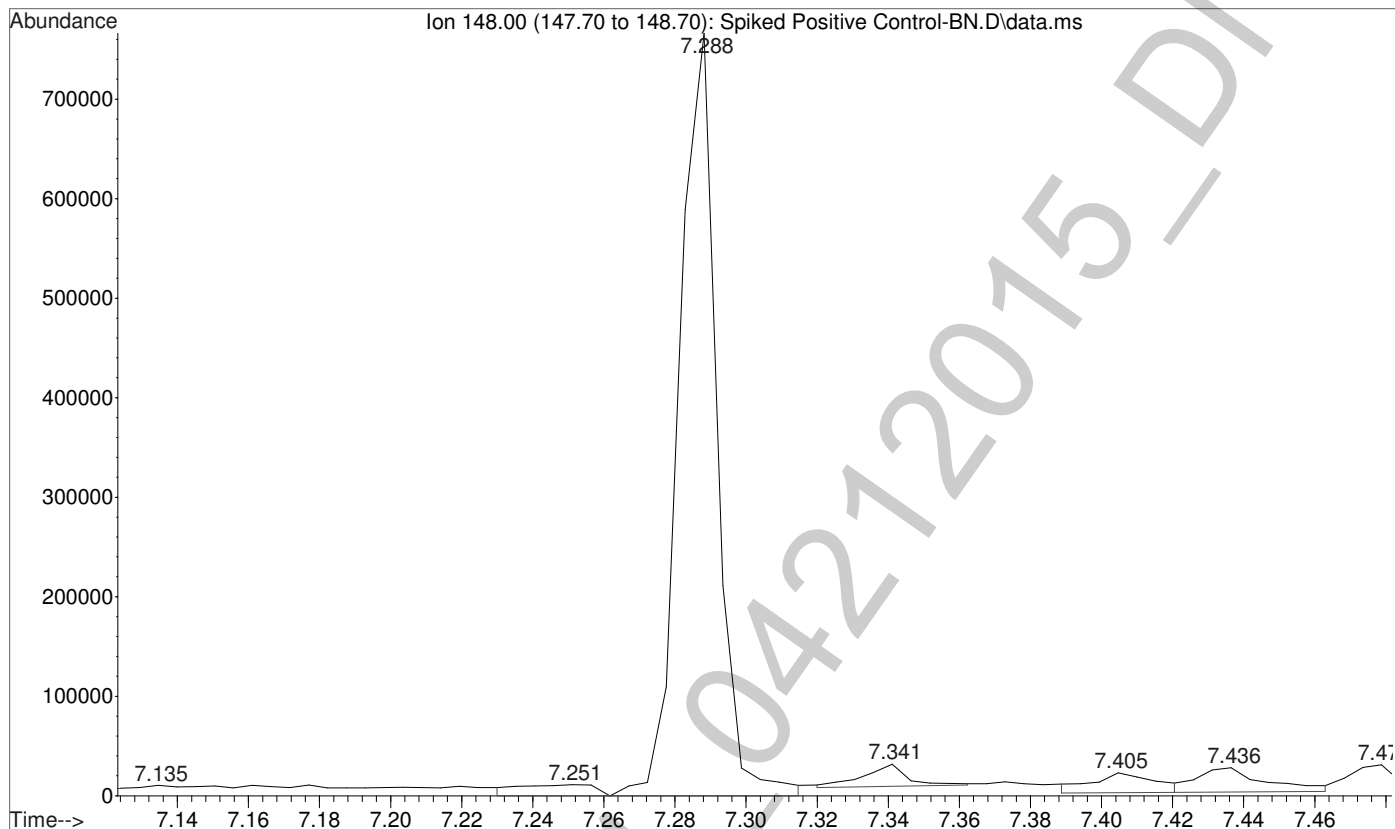



File :C:\gcms\1\data\Blood\042115BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 21 Apr 2015 12:07 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

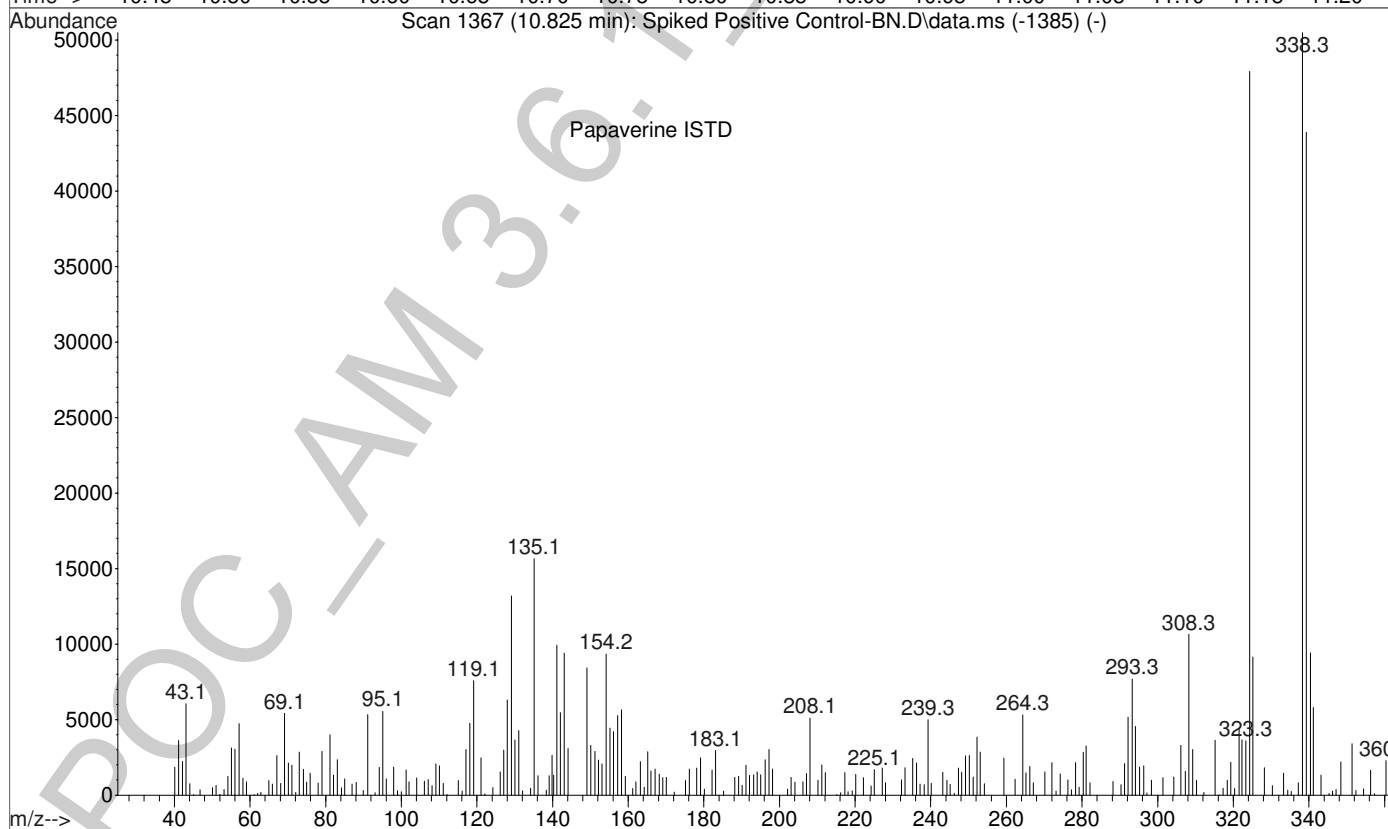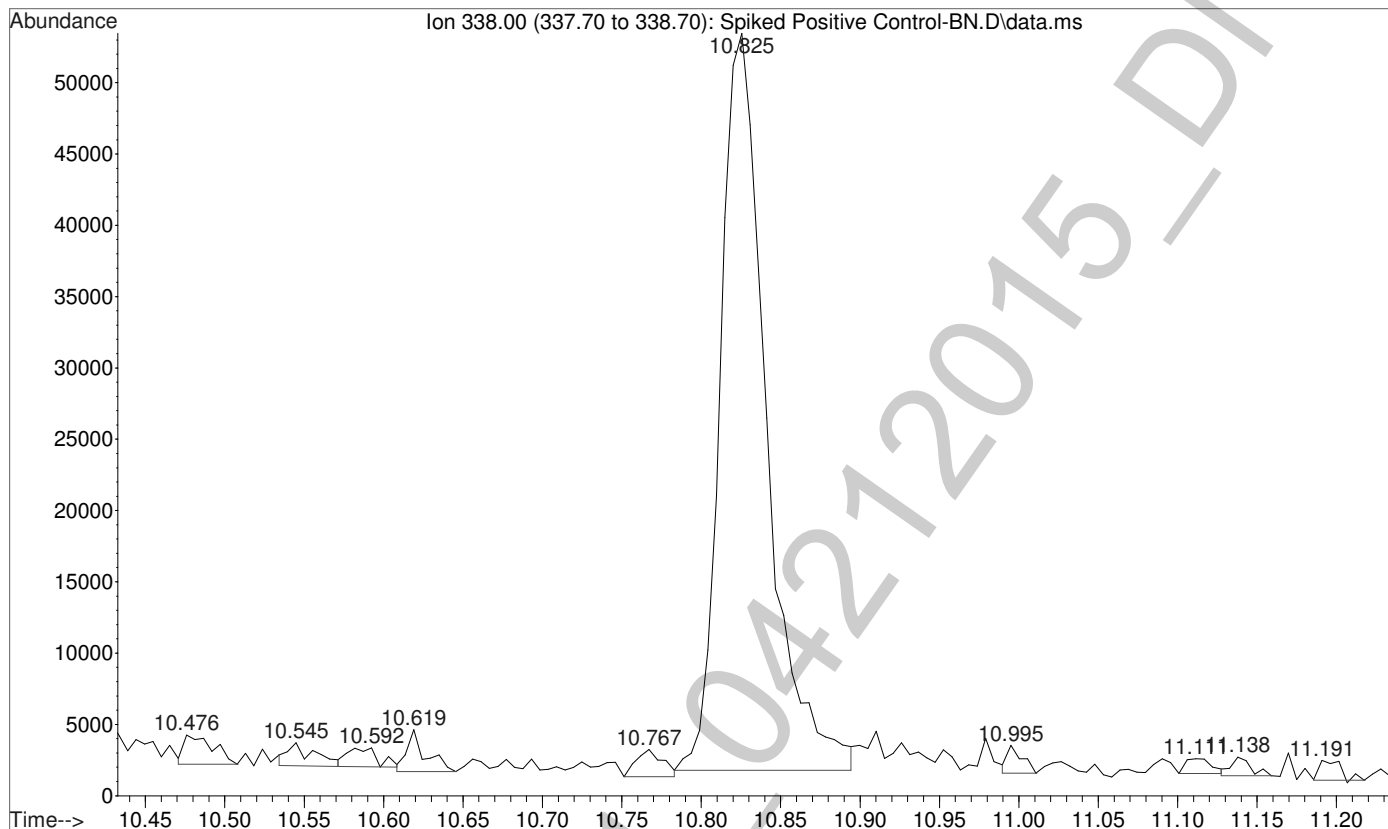



File :C:\gcms\1\data\Blood\042115BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 21 Apr 2015 12:07 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

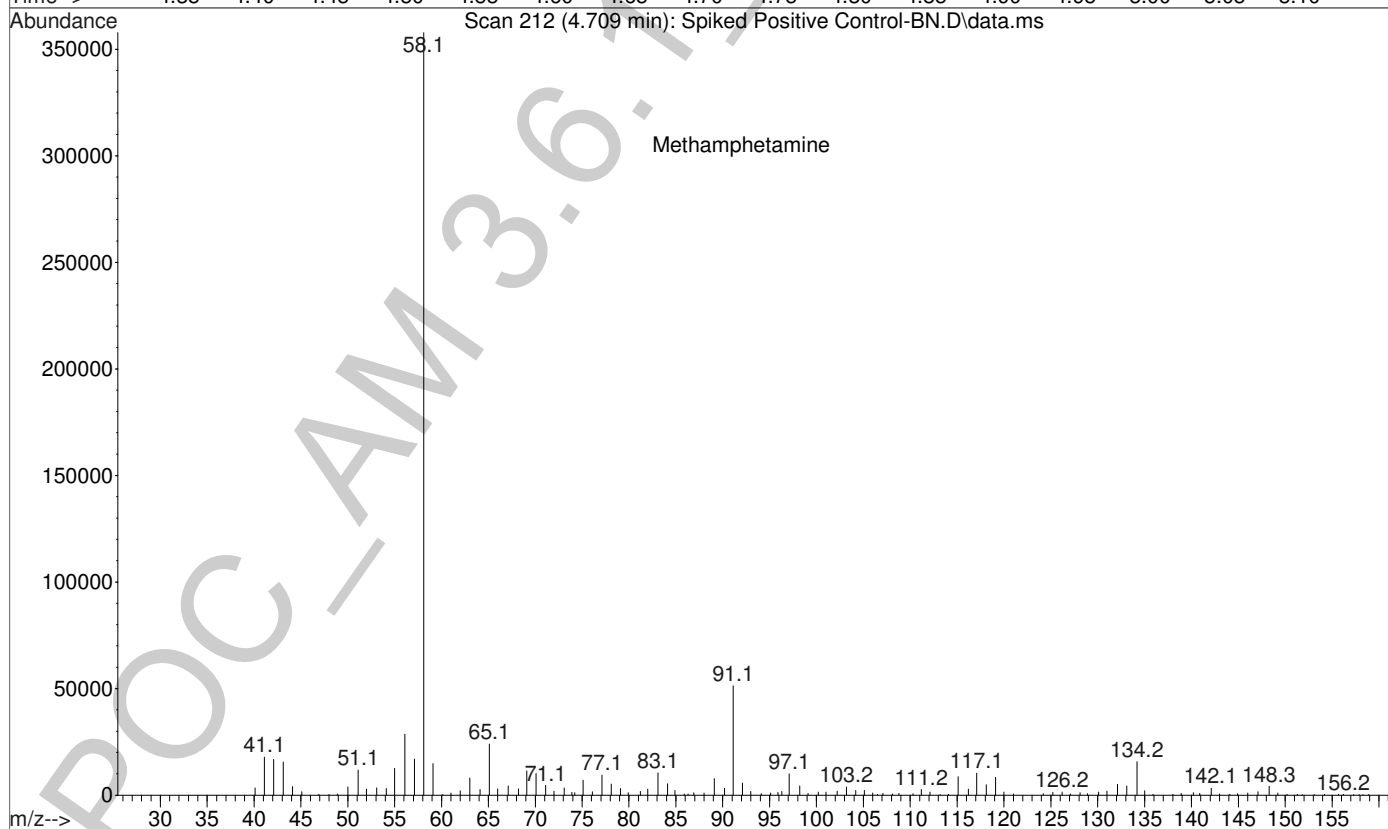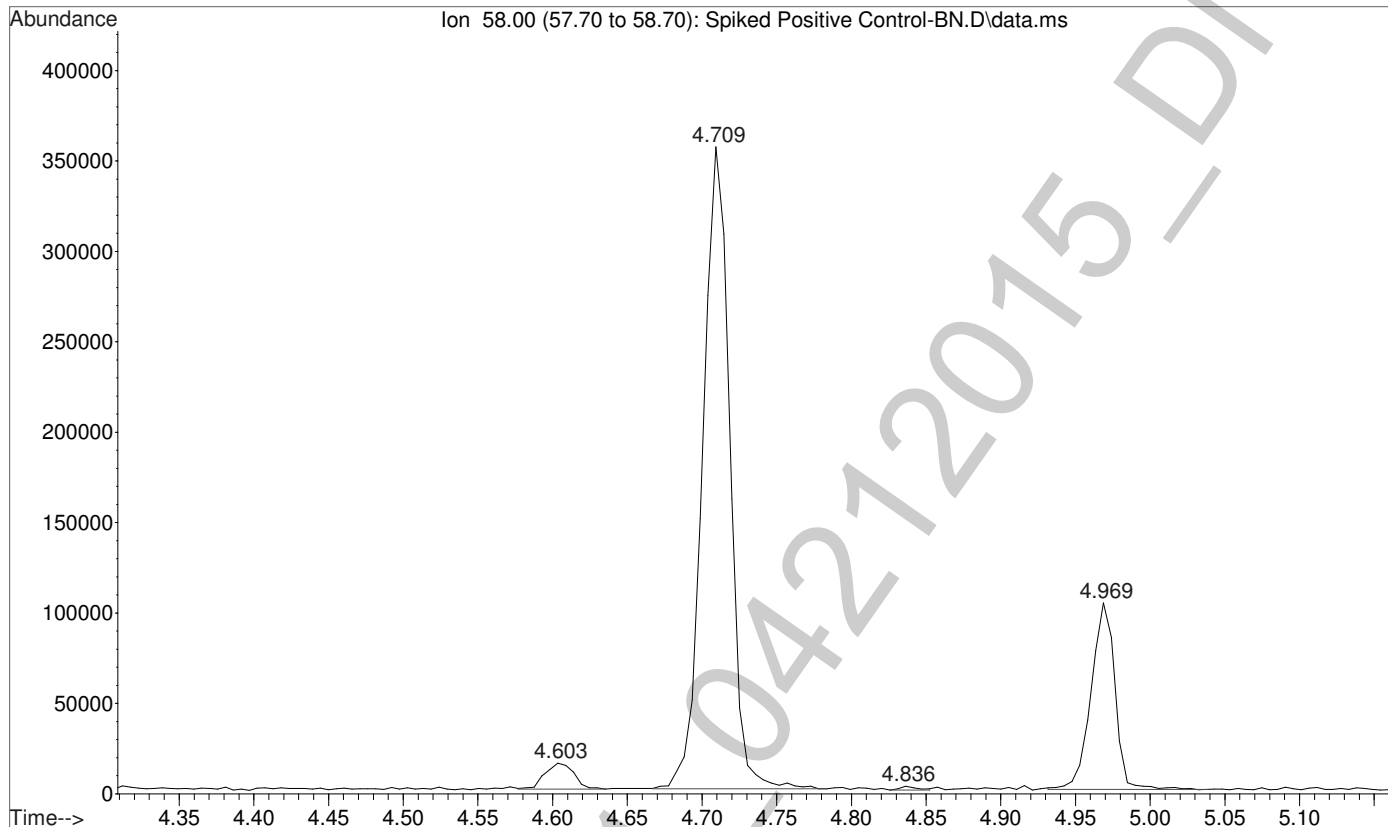



File :C:\gcms\1\data\Blood\042115BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 21 Apr 2015 12:07 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

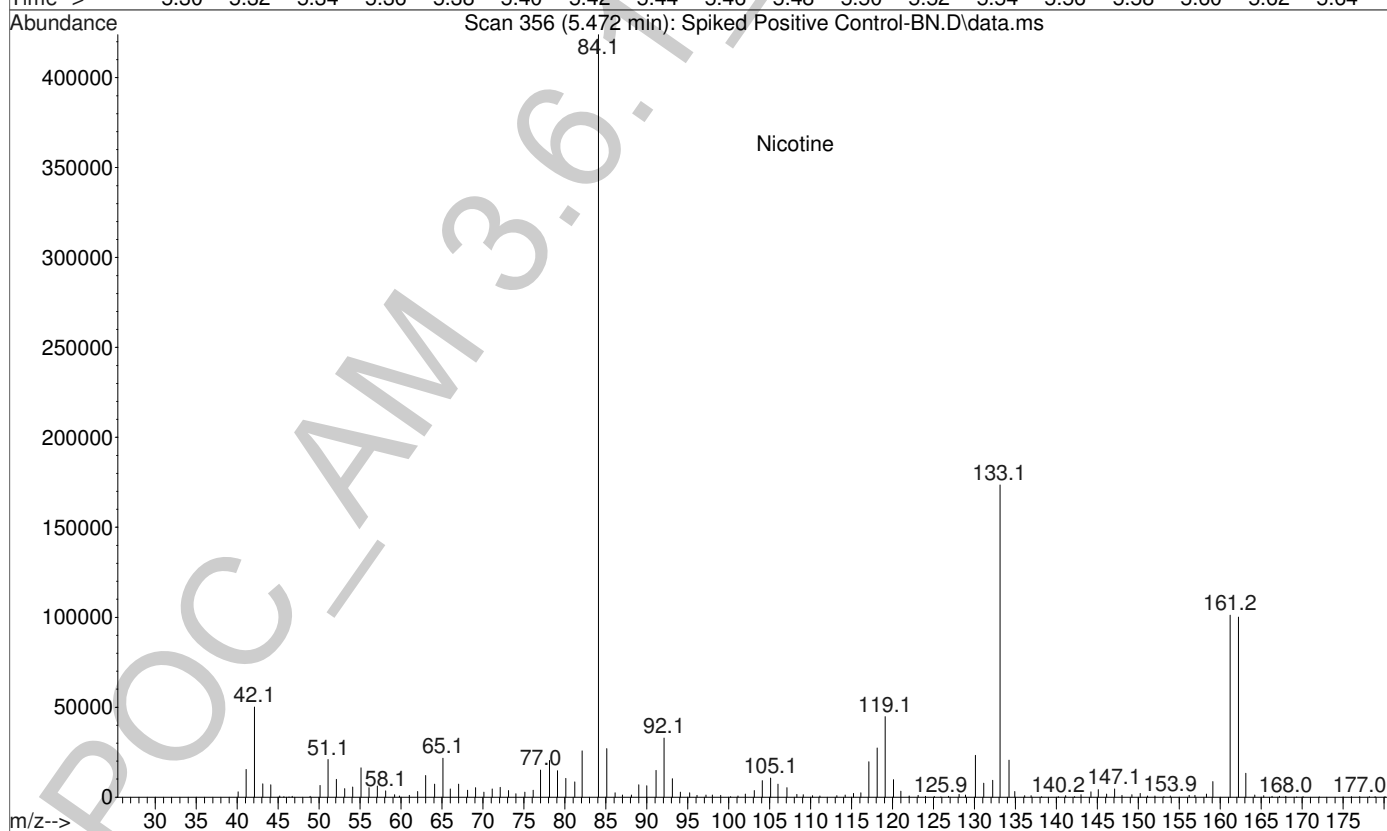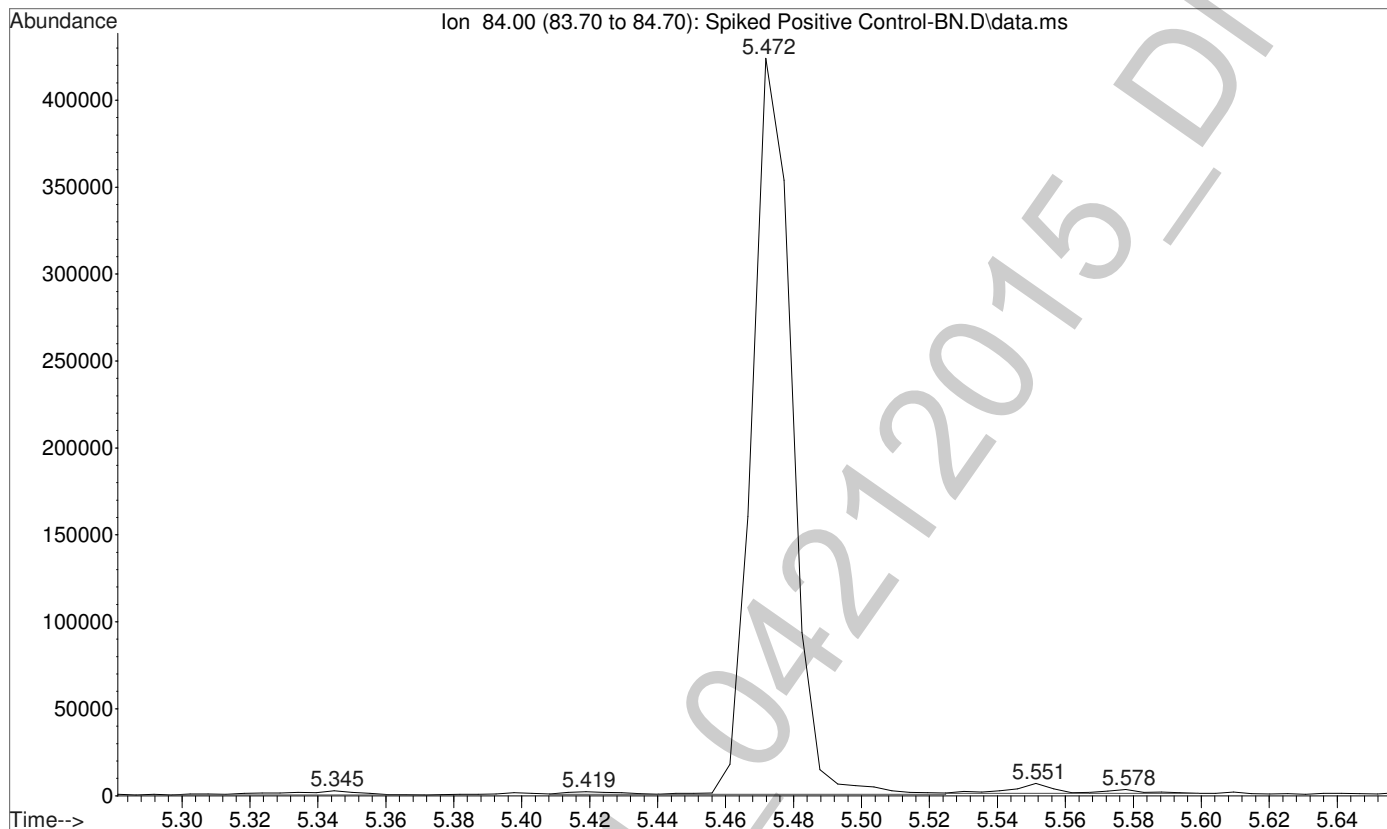



File :C:\gcms\1\data\Blood\042115BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 21 Apr 2015 12:07 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

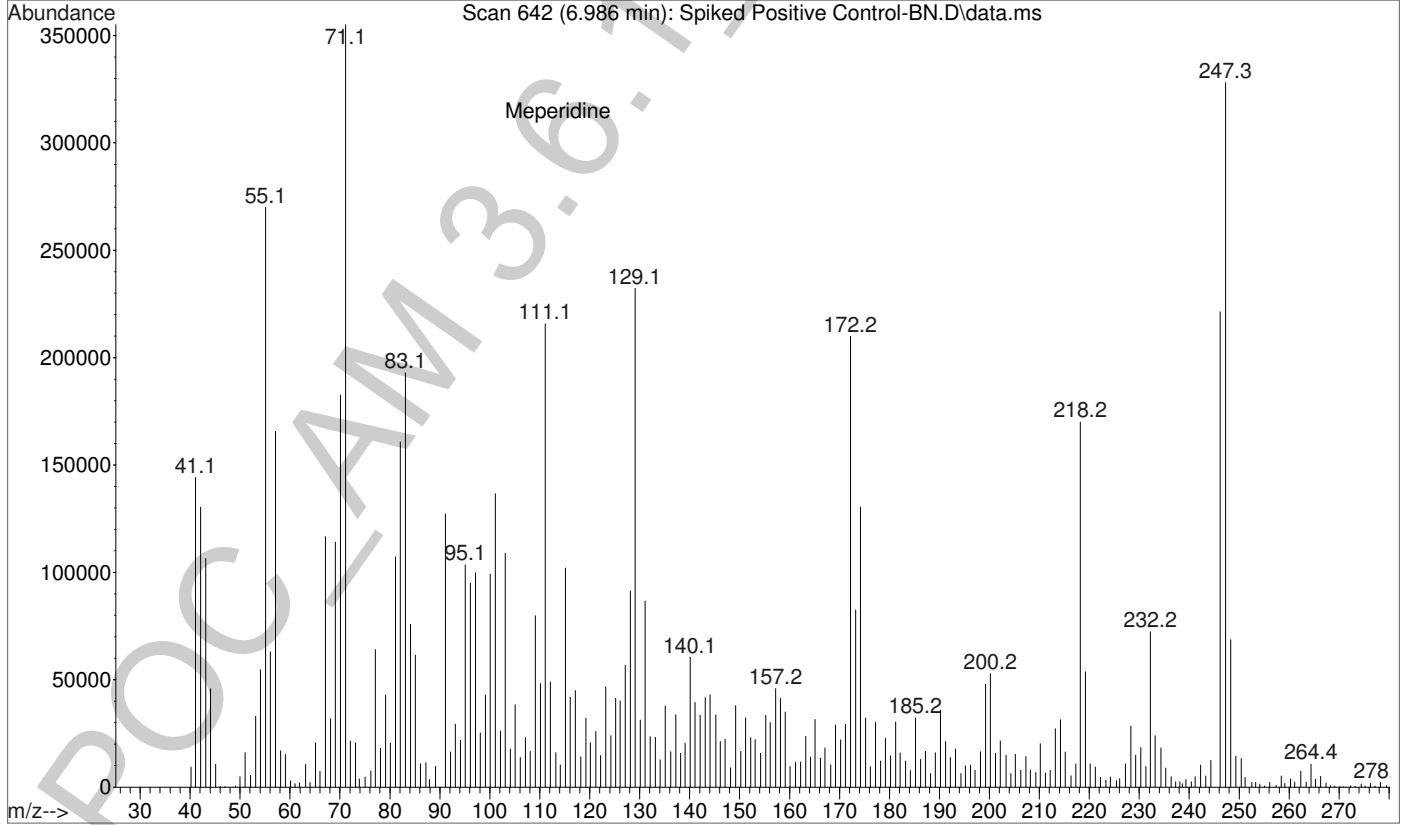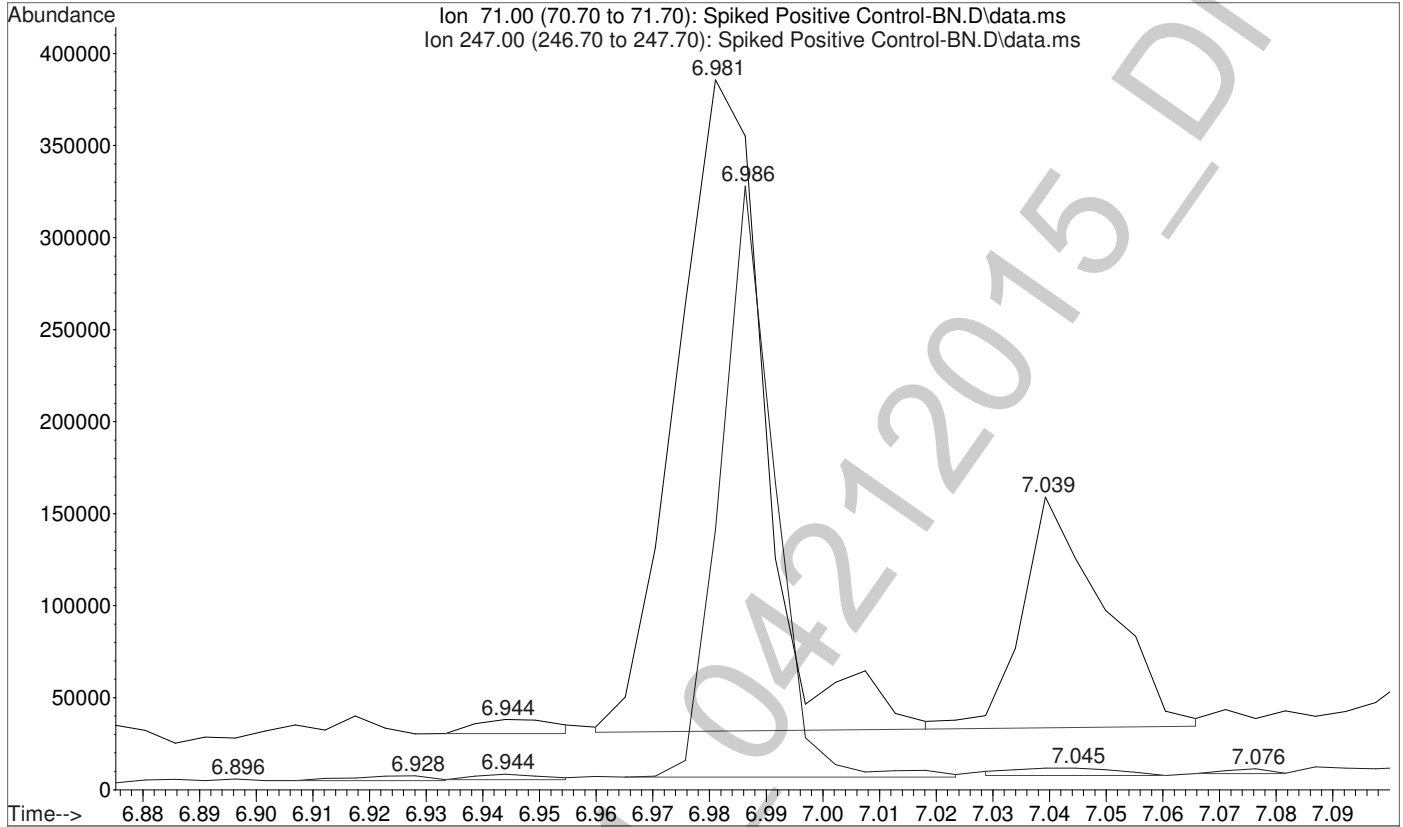



File :C:\gcms\1\data\Blood\042115BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 21 Apr 2015 12:07 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

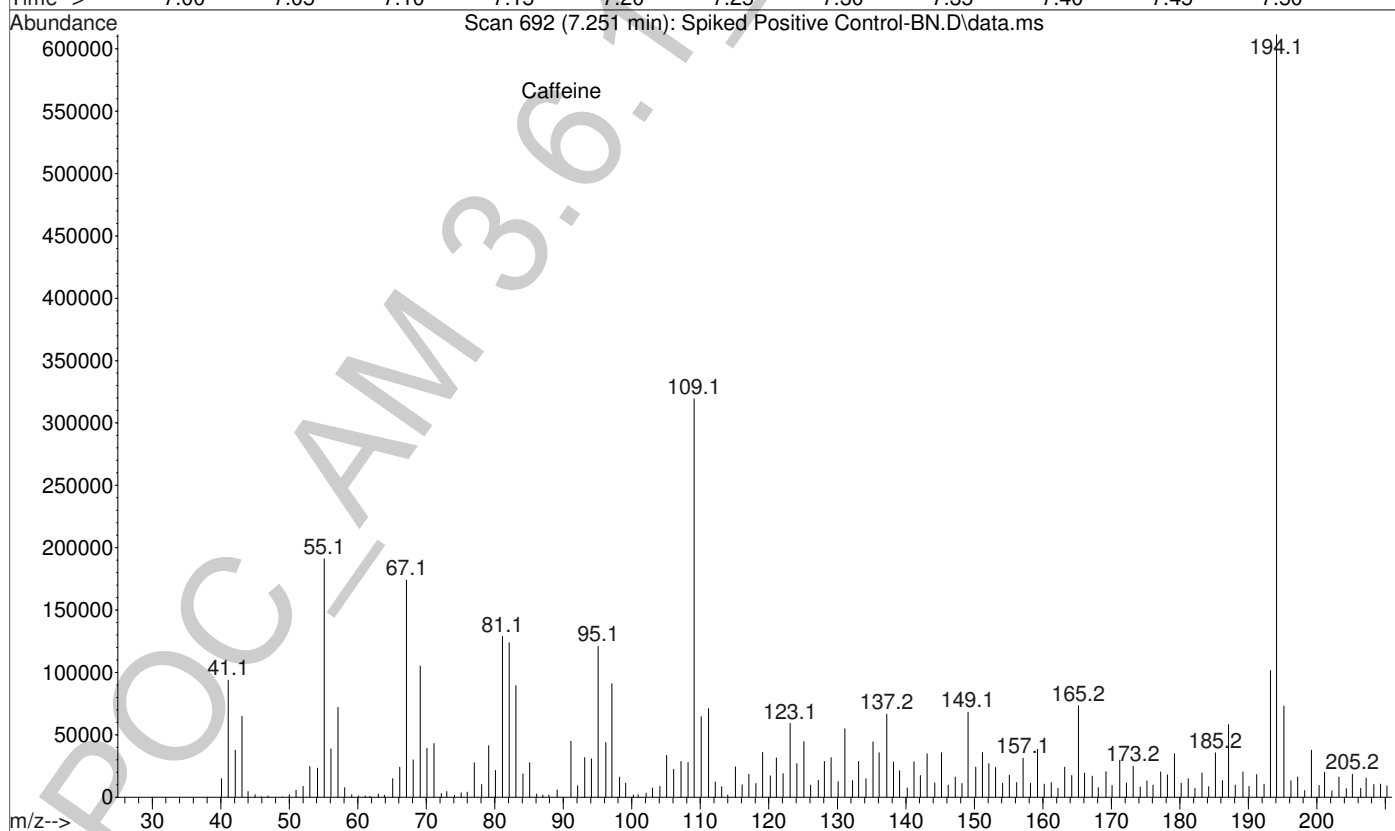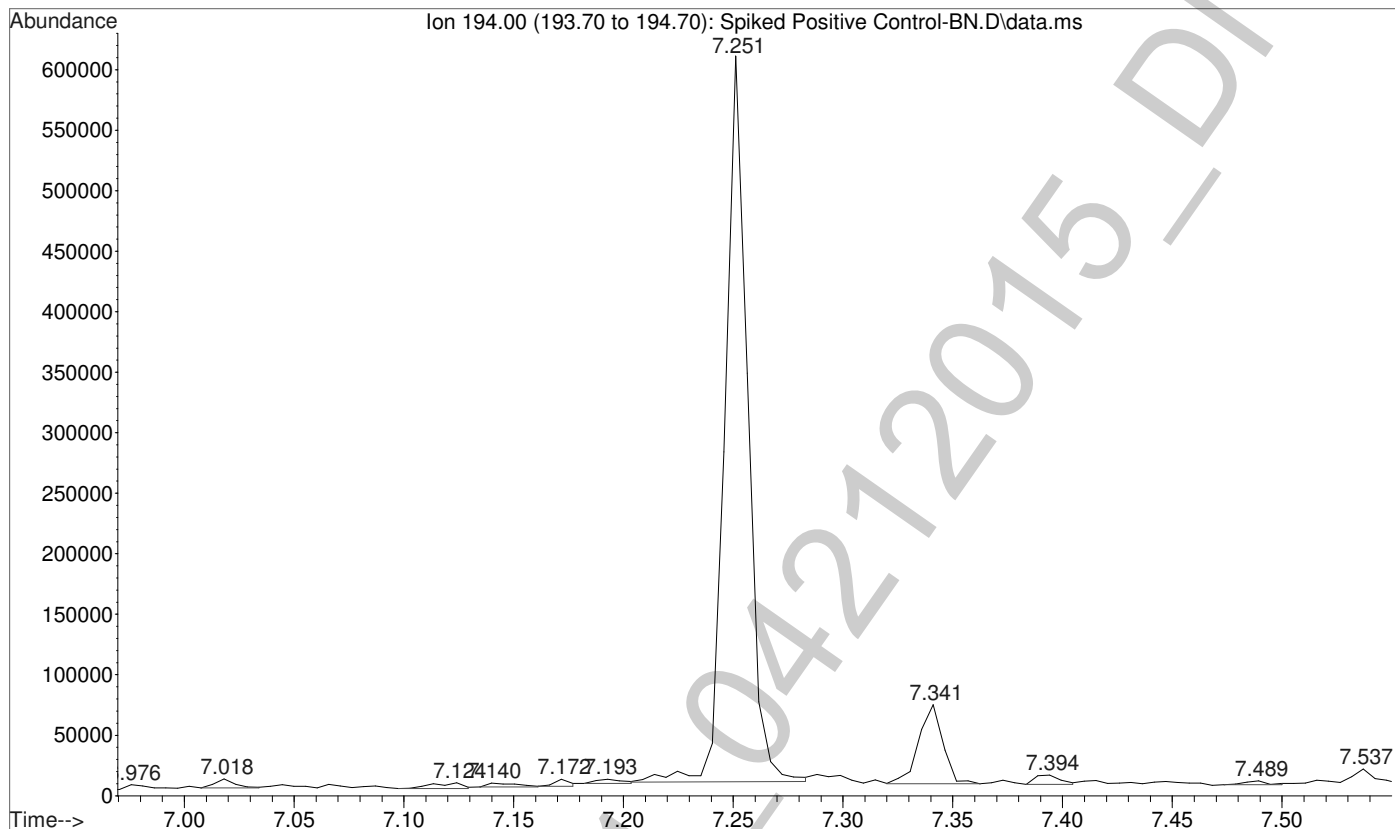



File :C:\gcms\1\data\Blood\042115BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 21 Apr 2015 12:07 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

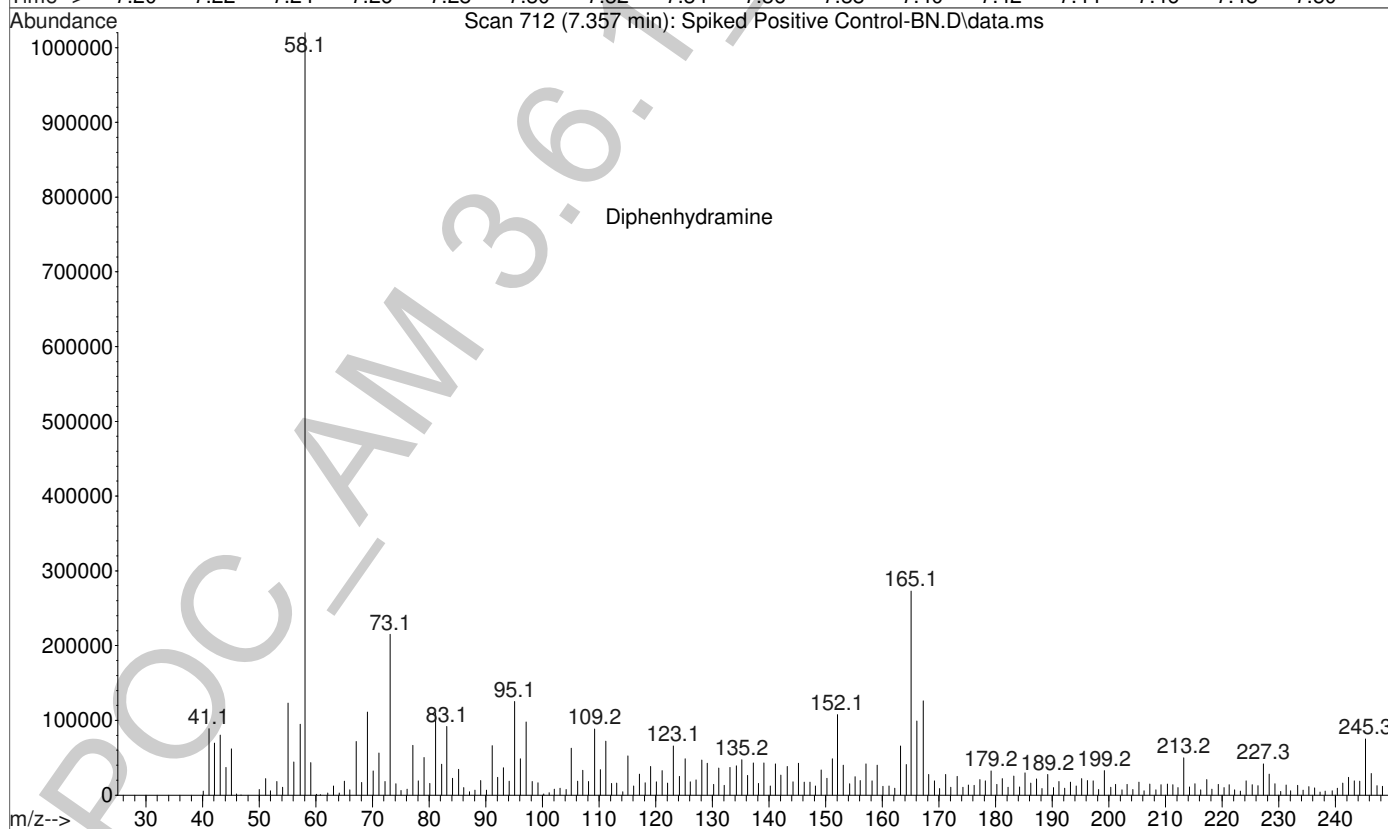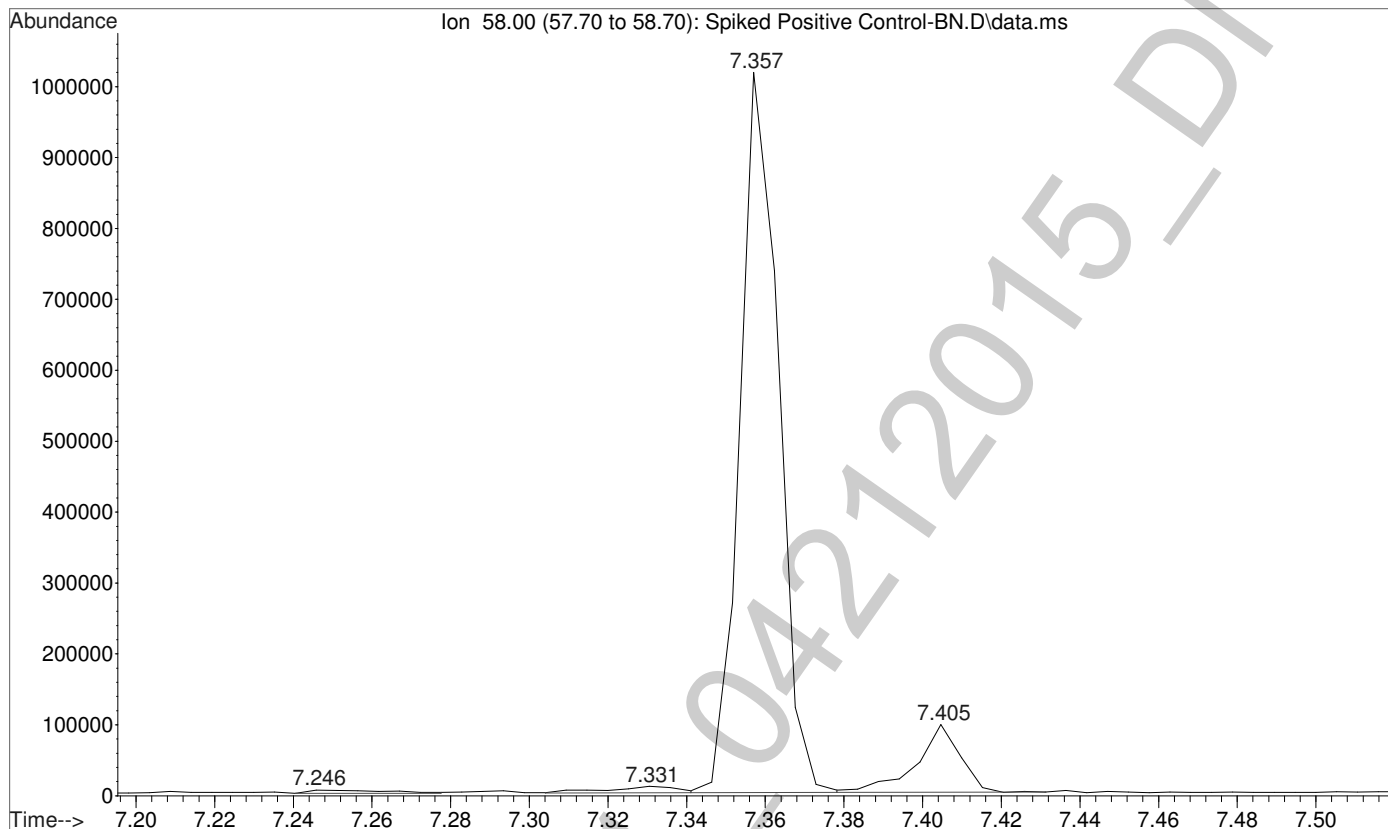



File :C:\gcms\1\data\Blood\042115BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 21 Apr 2015 12:07 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

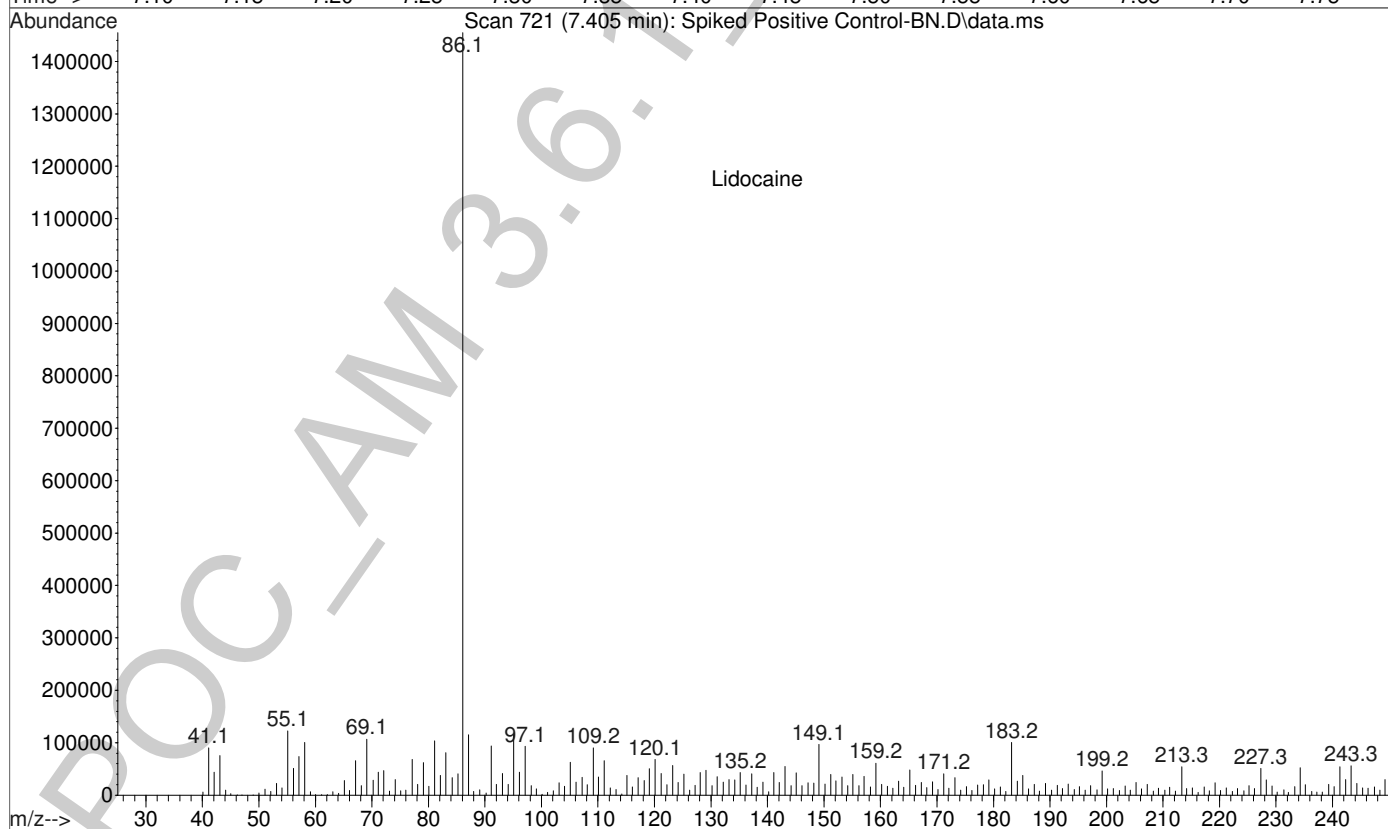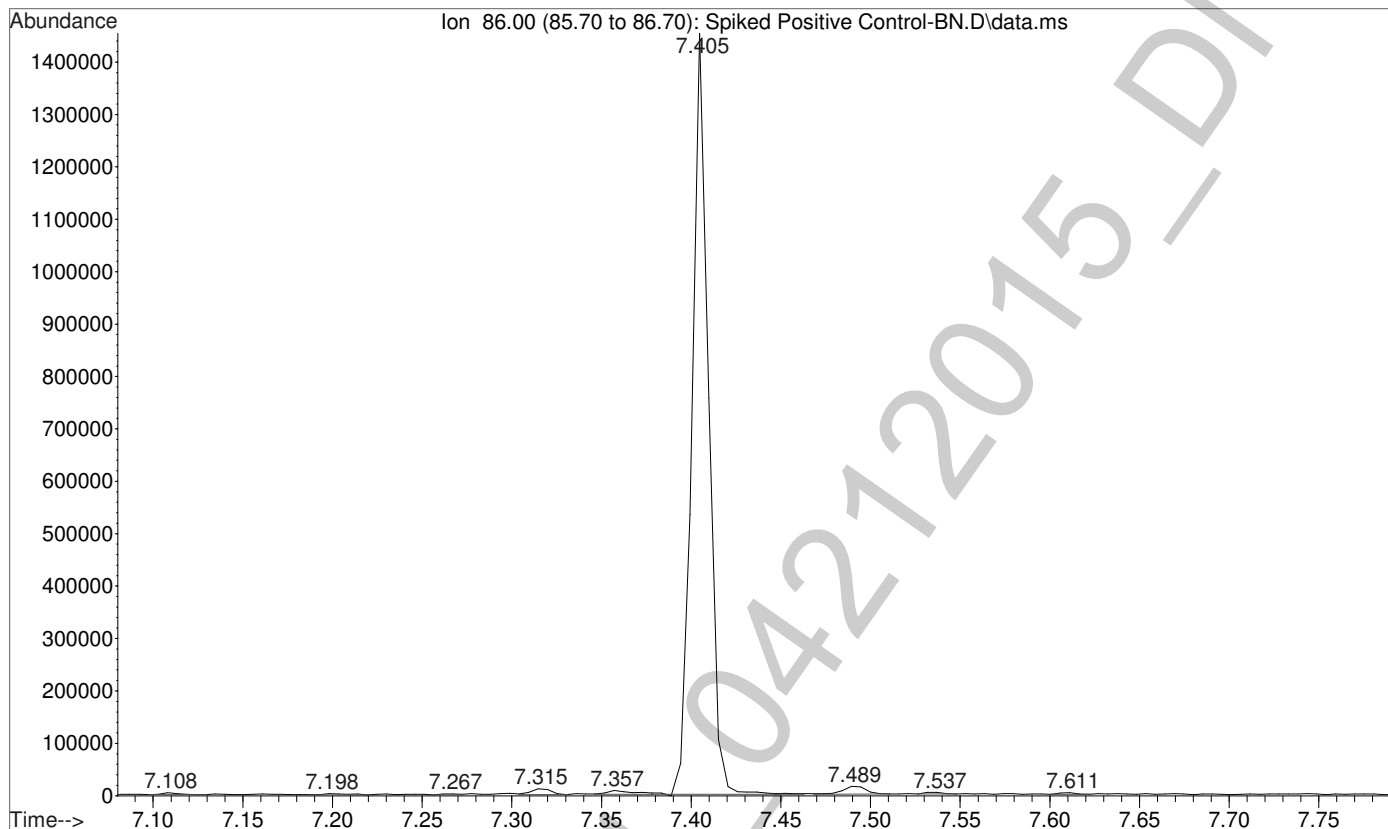



File :C:\gcms\1\data\Blood\042115BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 21 Apr 2015 12:07 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

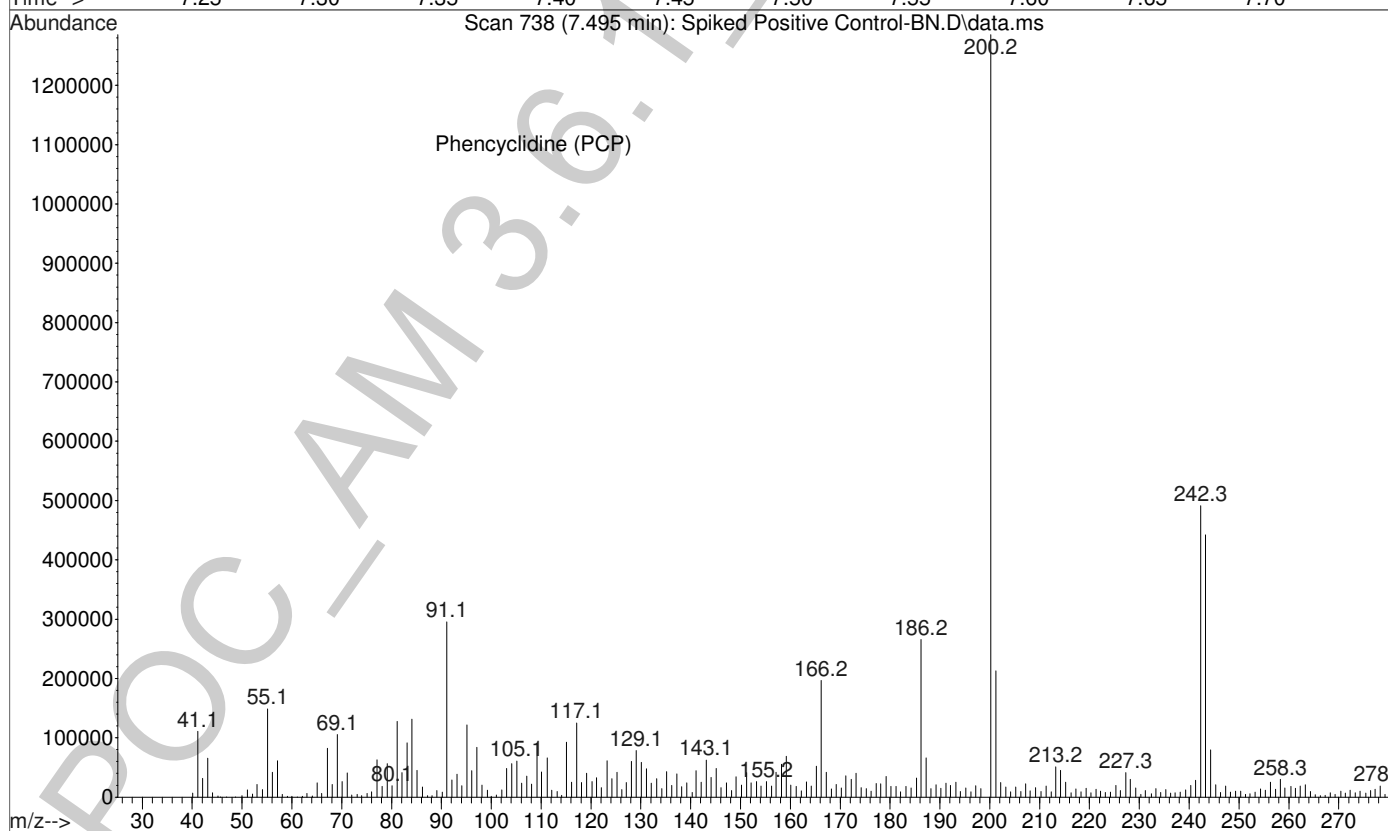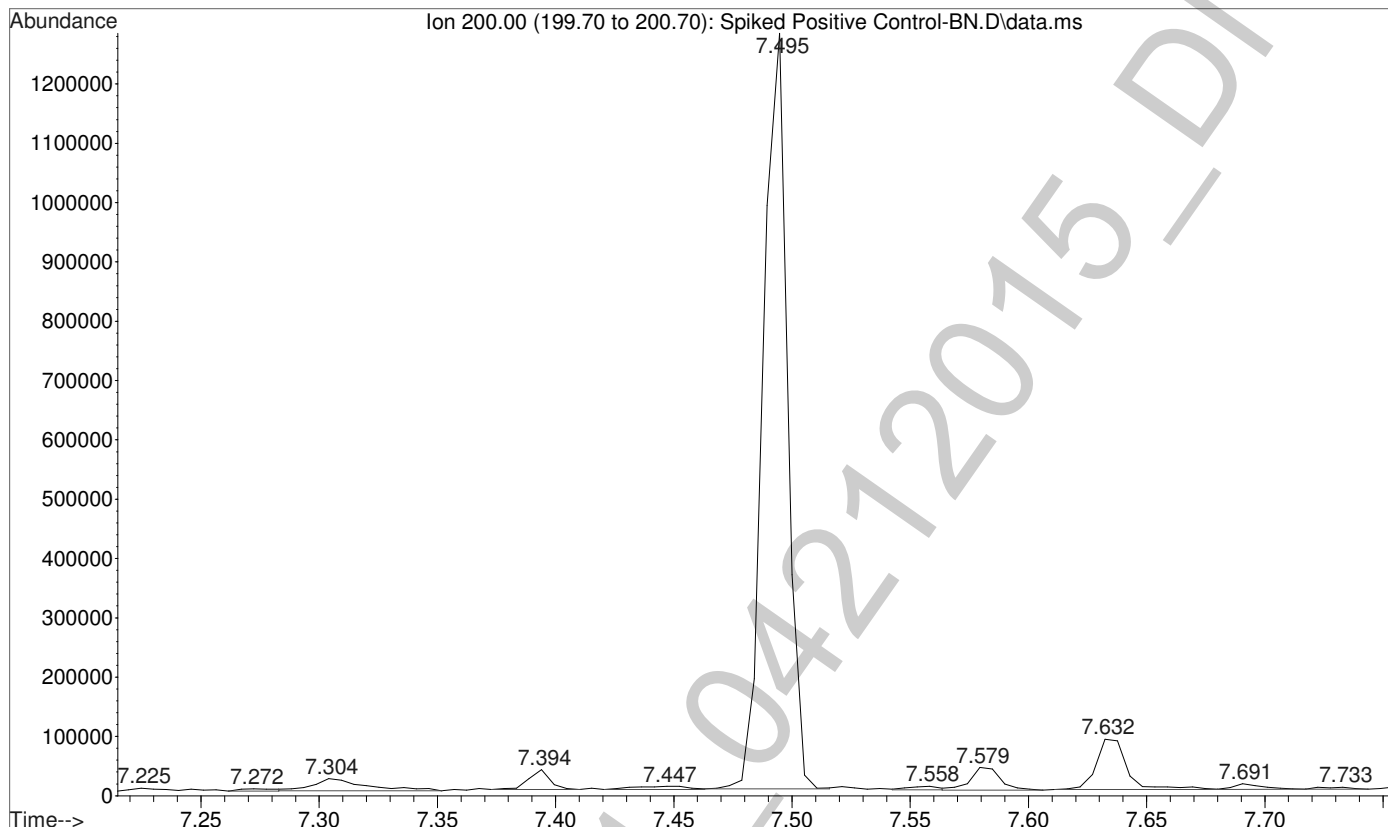



File :C:\gcms\1\data\Blood\042115BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 21 Apr 2015 12:07 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

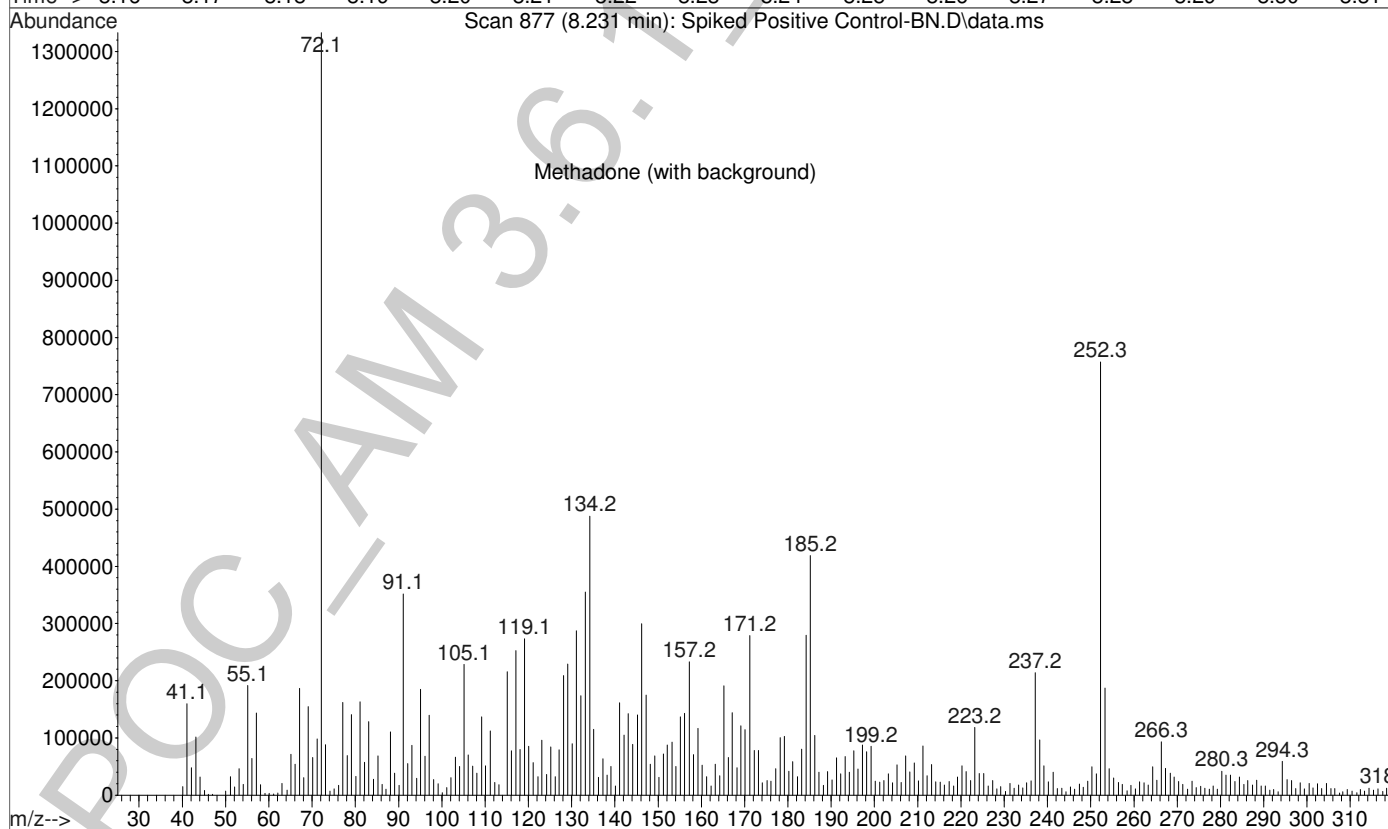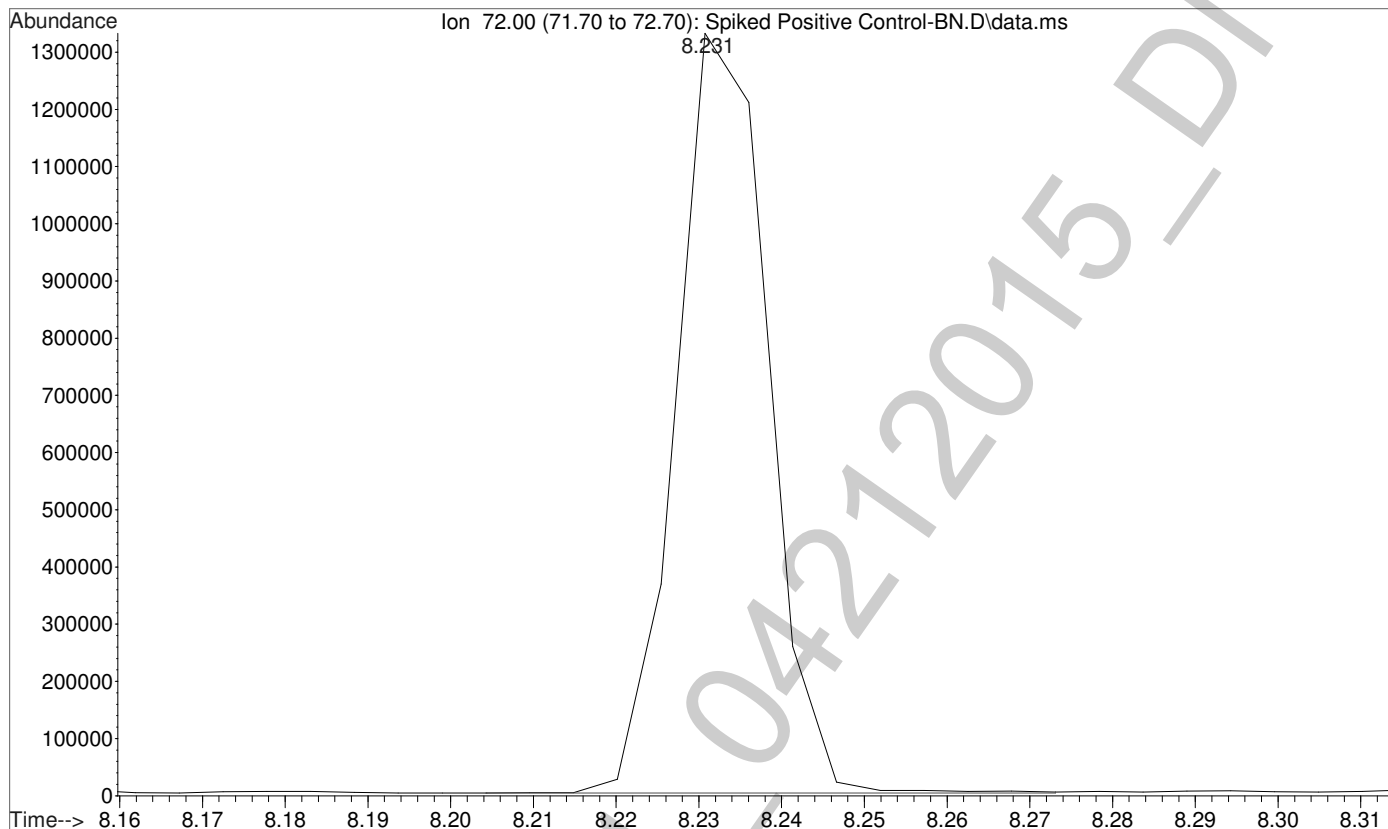



File :C:\gcms\1\data\Blood\042115BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 21 Apr 2015 12:07 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

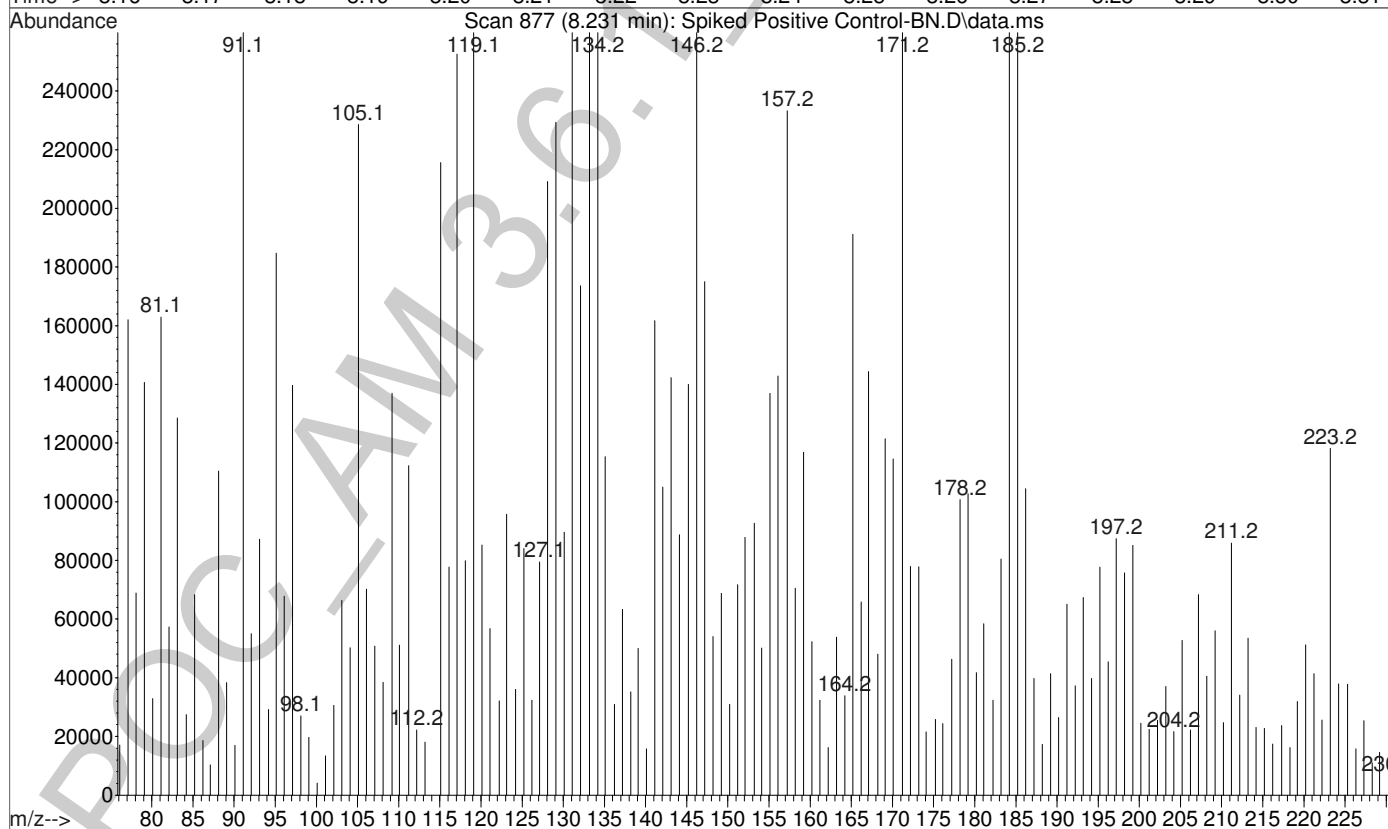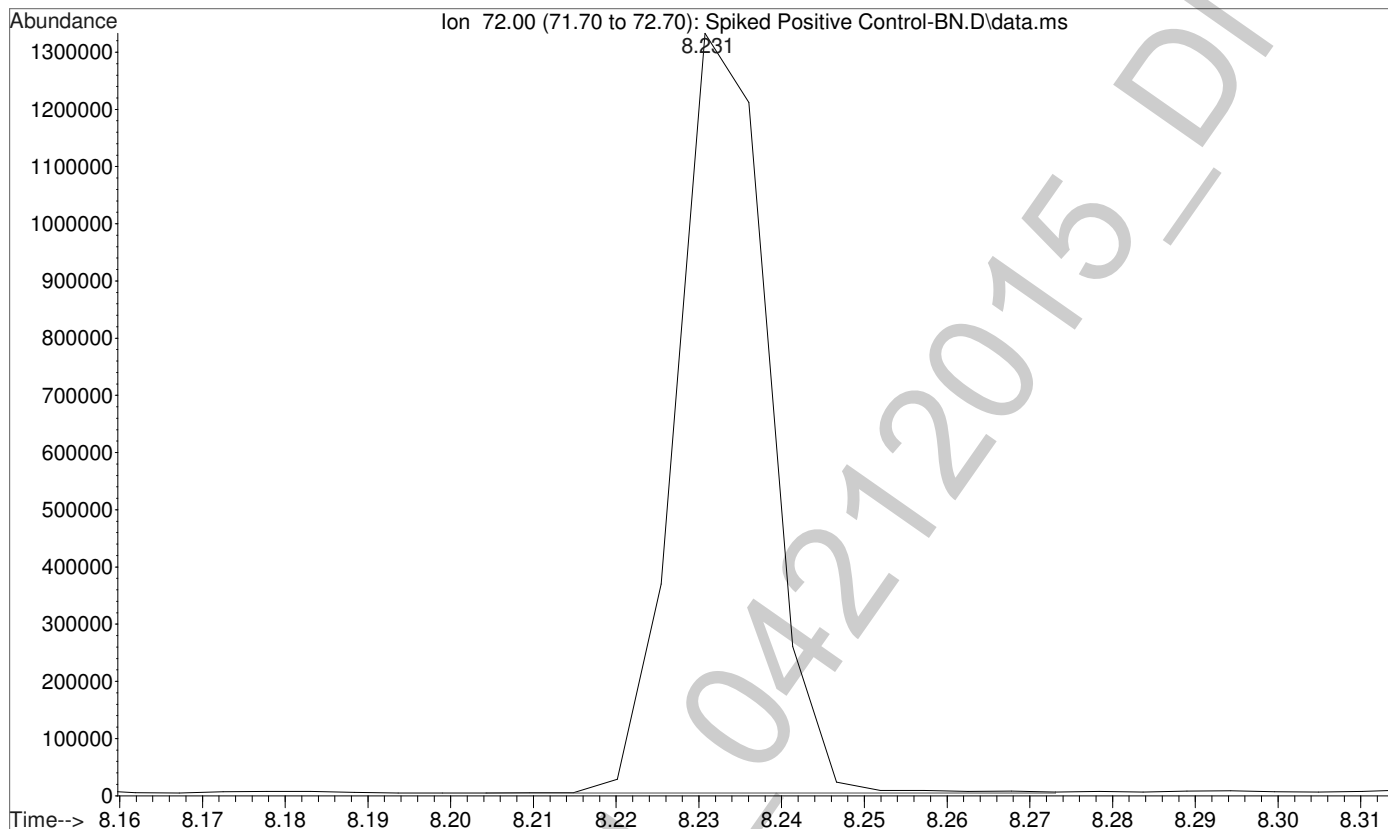



File :C:\gcms\1\data\Blood\042115BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 21 Apr 2015 12:07 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

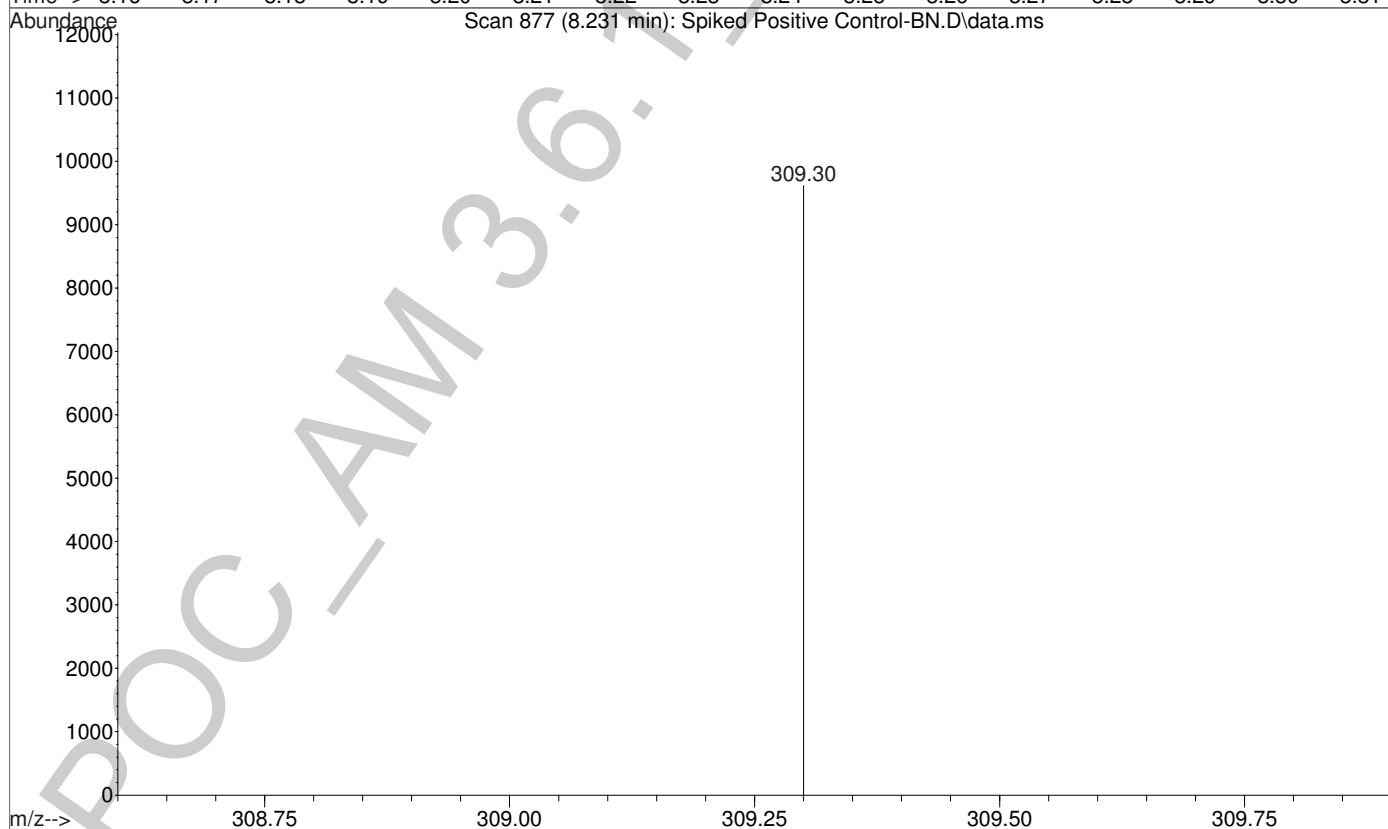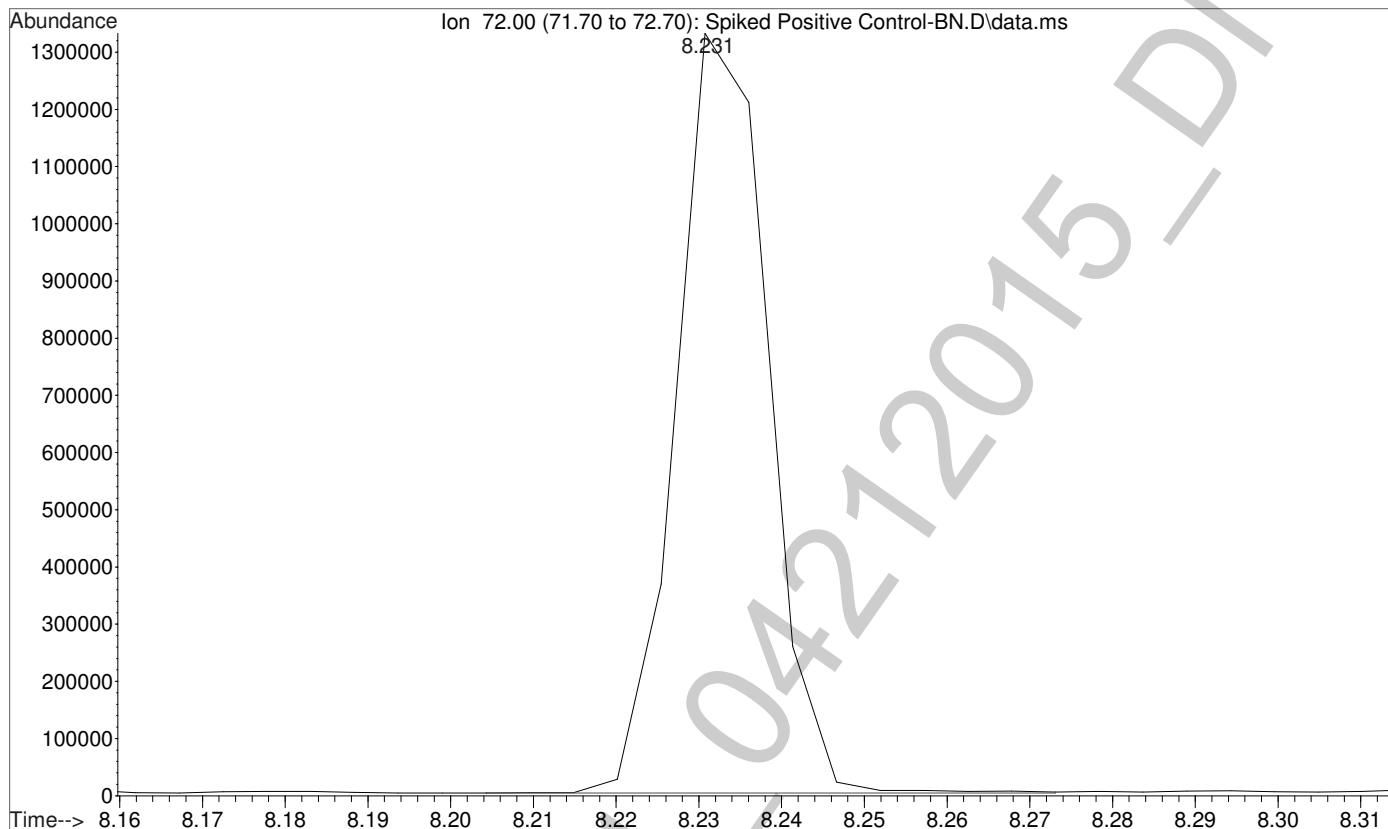



File :C:\gcms\1\data\Blood\042115BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 21 Apr 2015 12:07 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

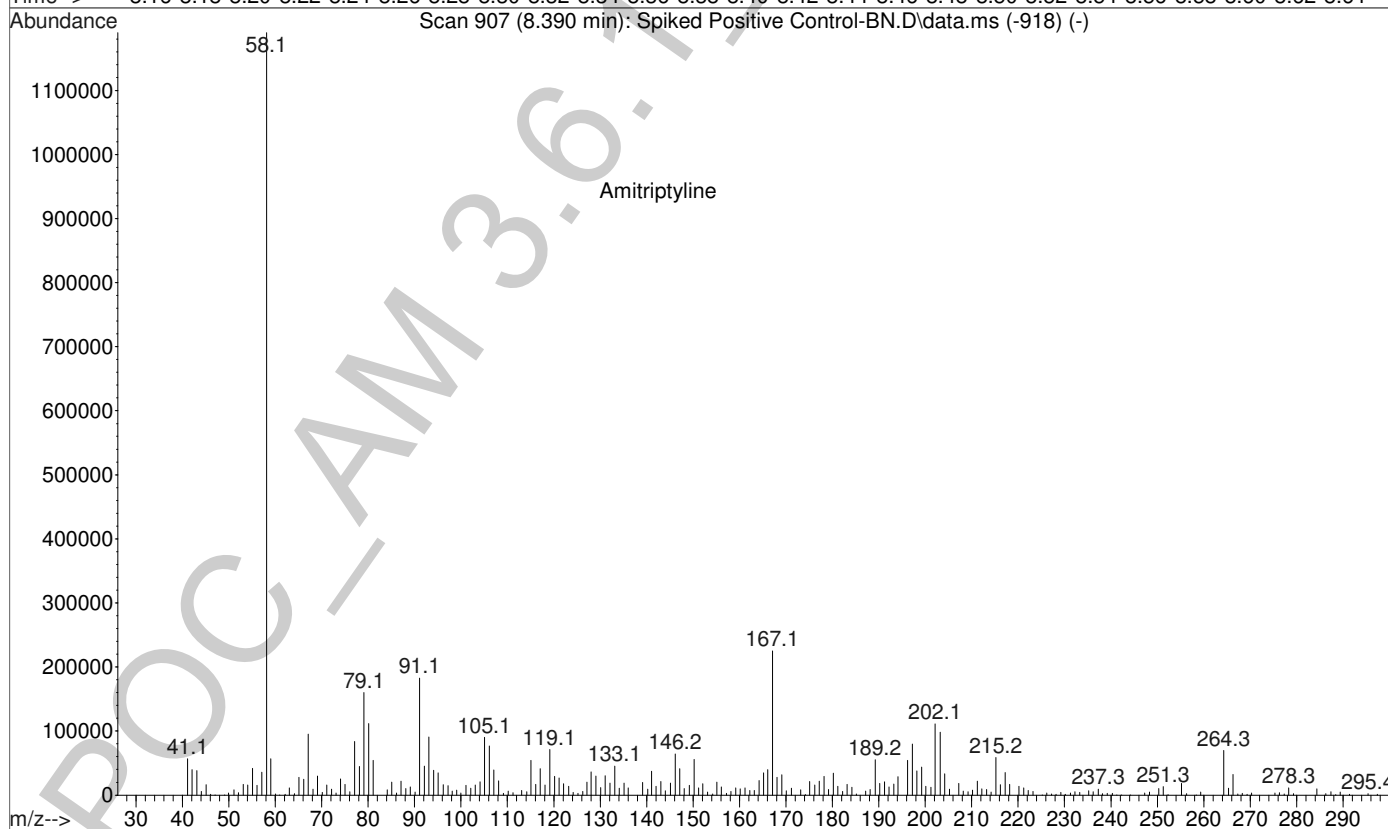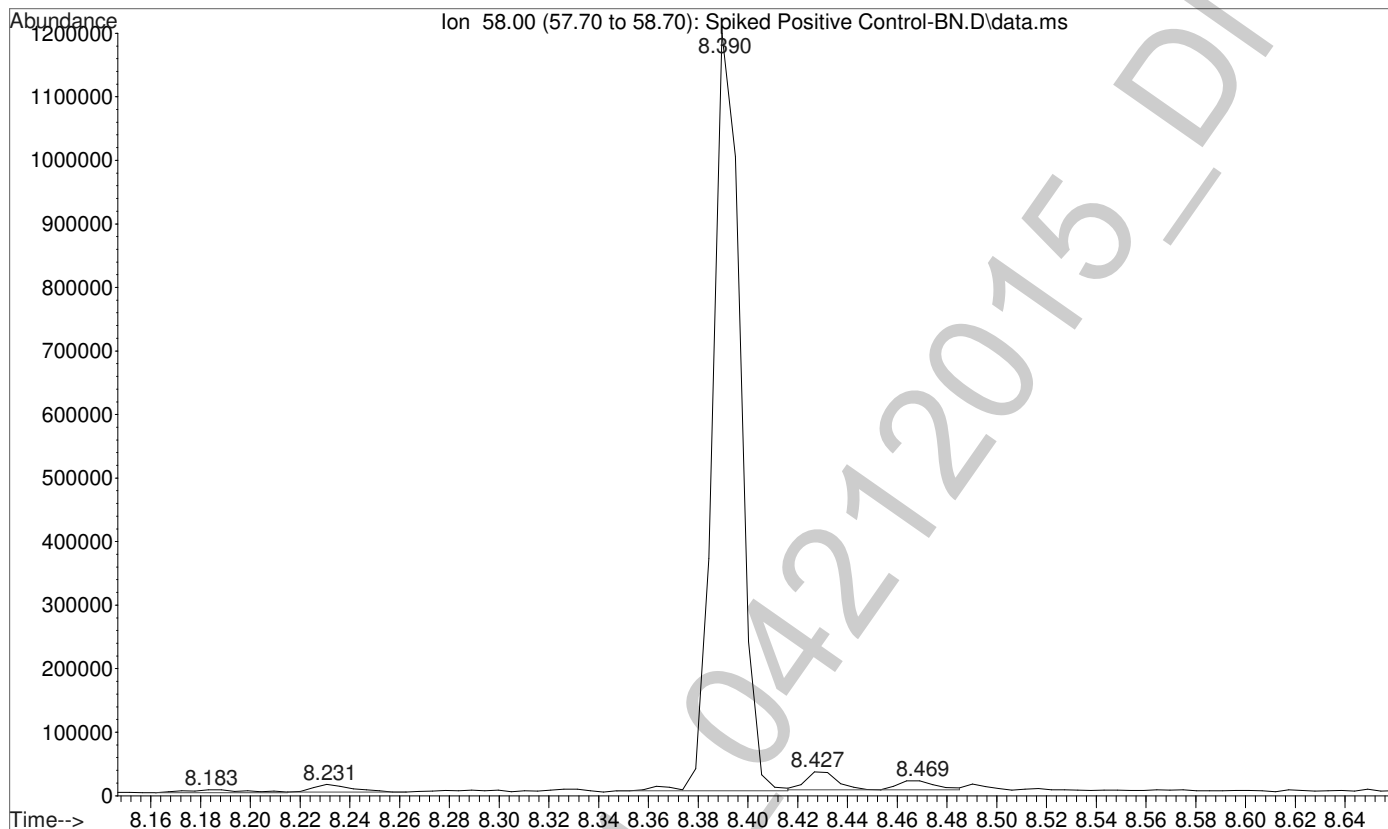



File :C:\gcms\1\data\Blood\042115BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 21 Apr 2015 12:07 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

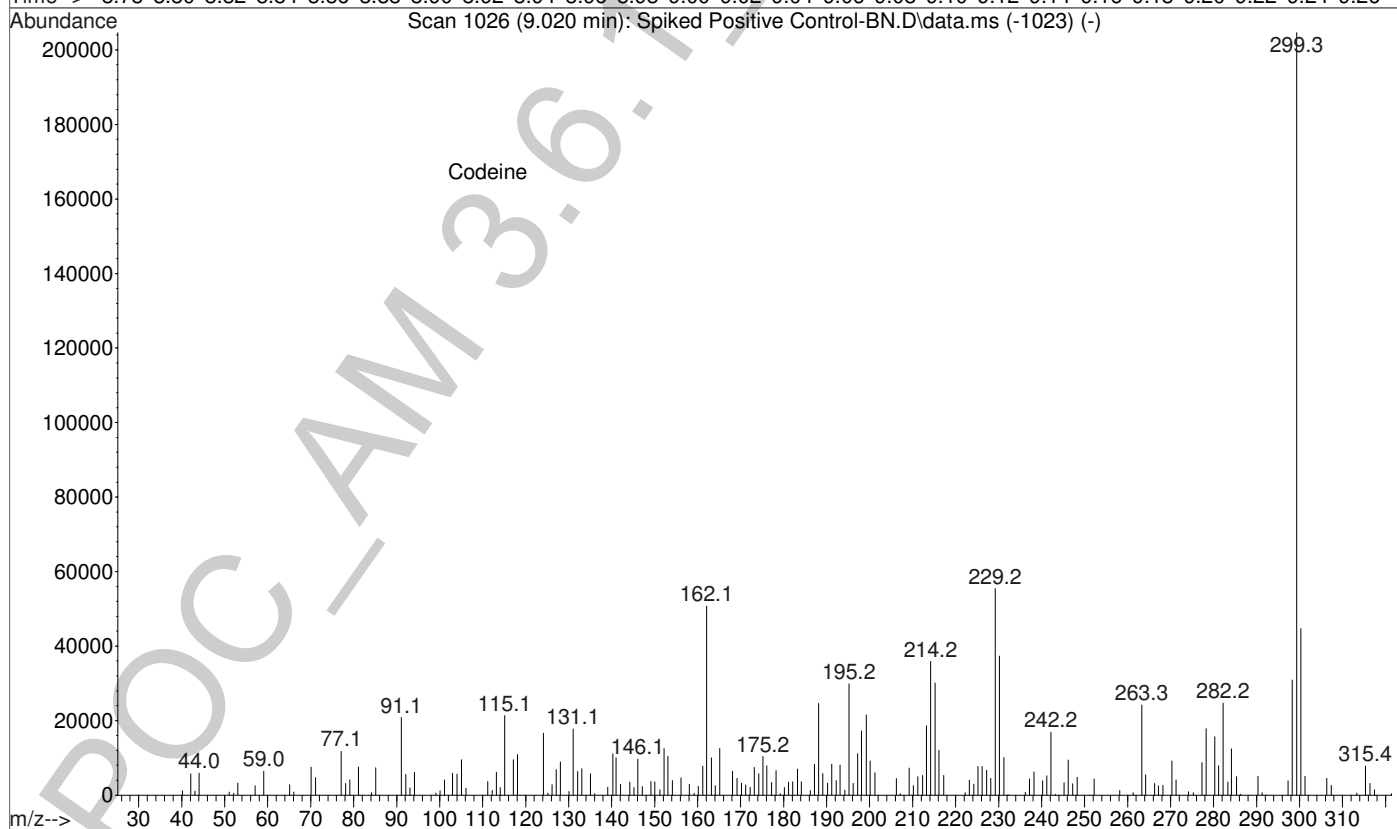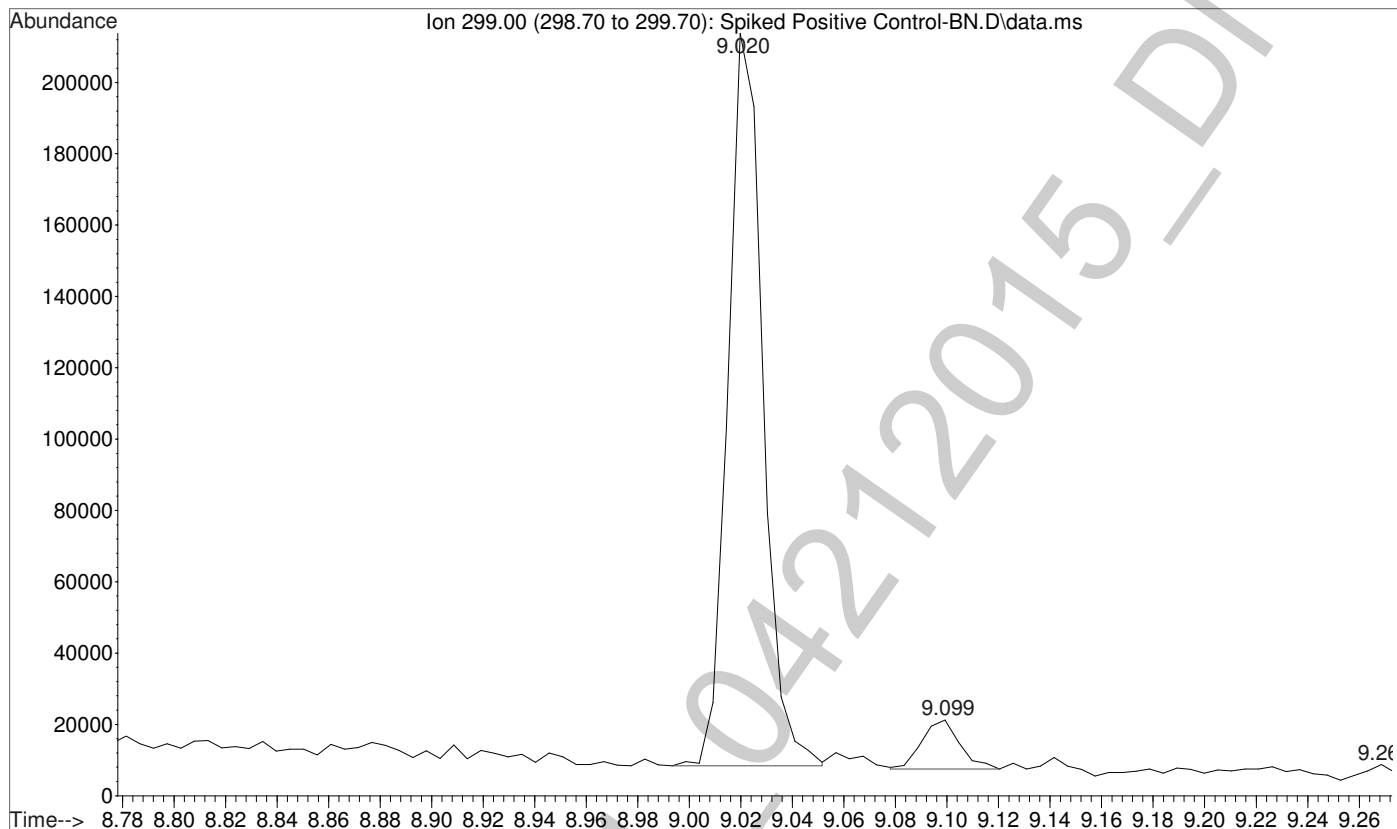

File :C:\gcms\1\data\Blood\042115BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 21 Apr 2015 12:07 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

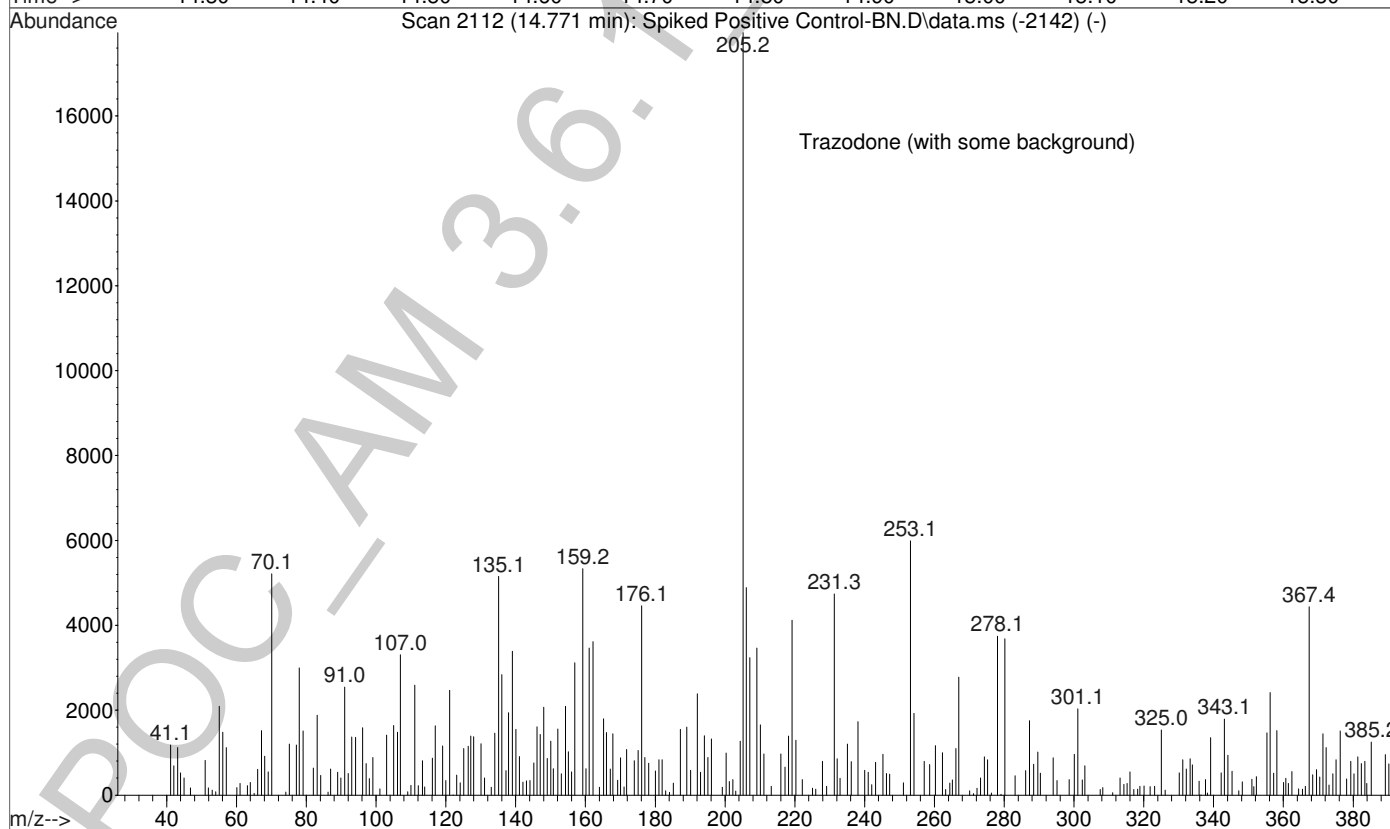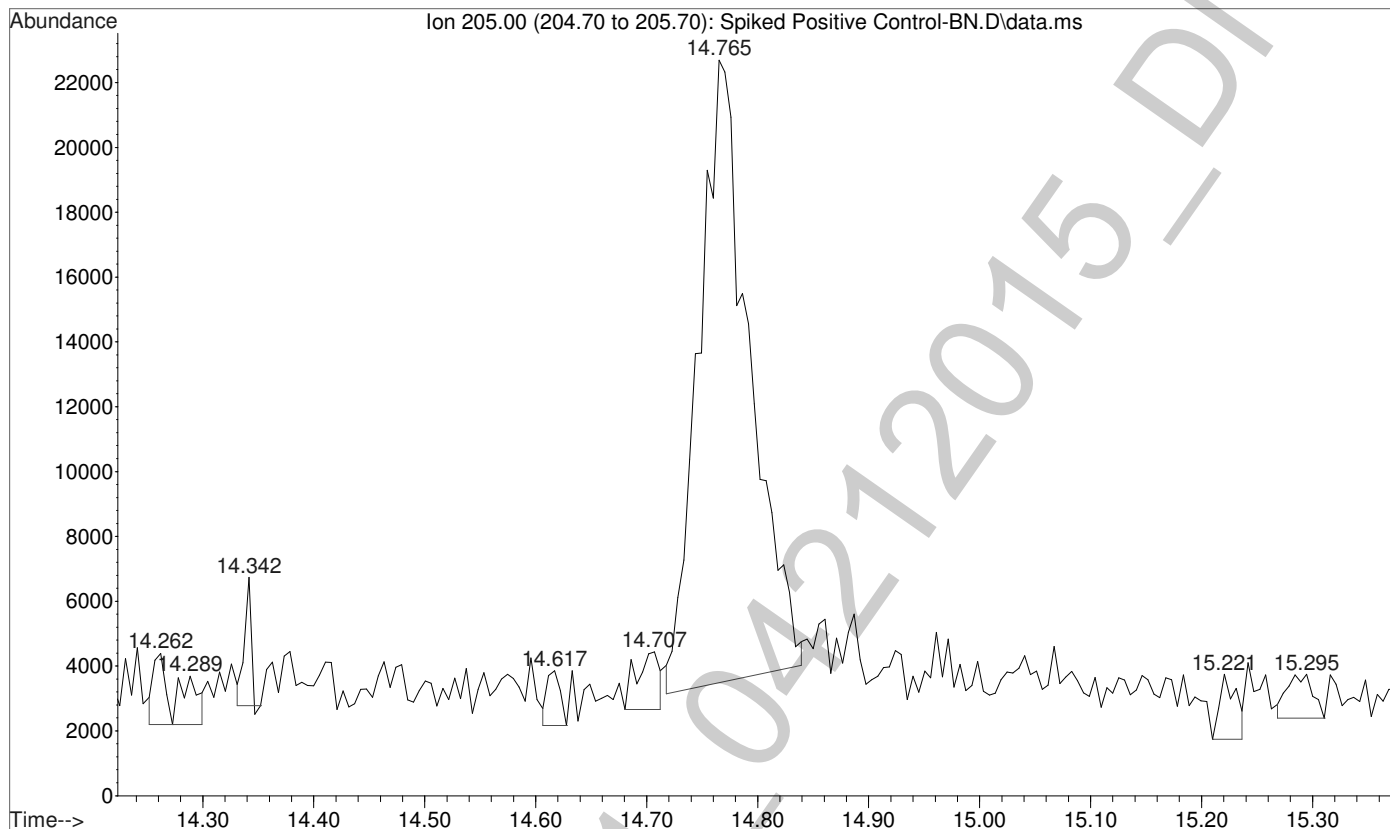

File :C:\gcms\1\data\Blood\042115BN\prbLK2.D
Operator : 5LAB-C01\ISPuser
Acquired : 21 Apr 2015 12:30 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Solvent Blank
Misc Info : Chloroform
Vial Number: 99

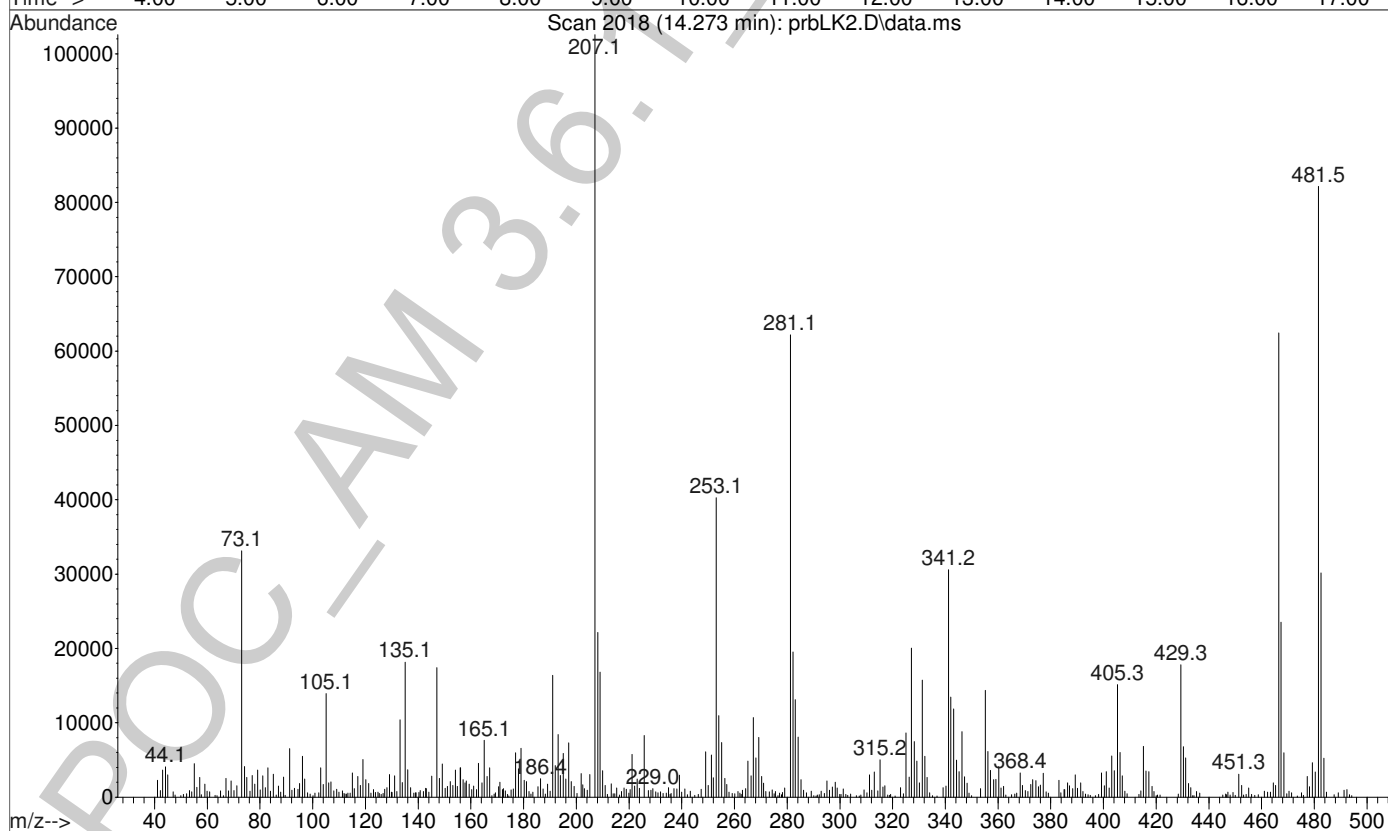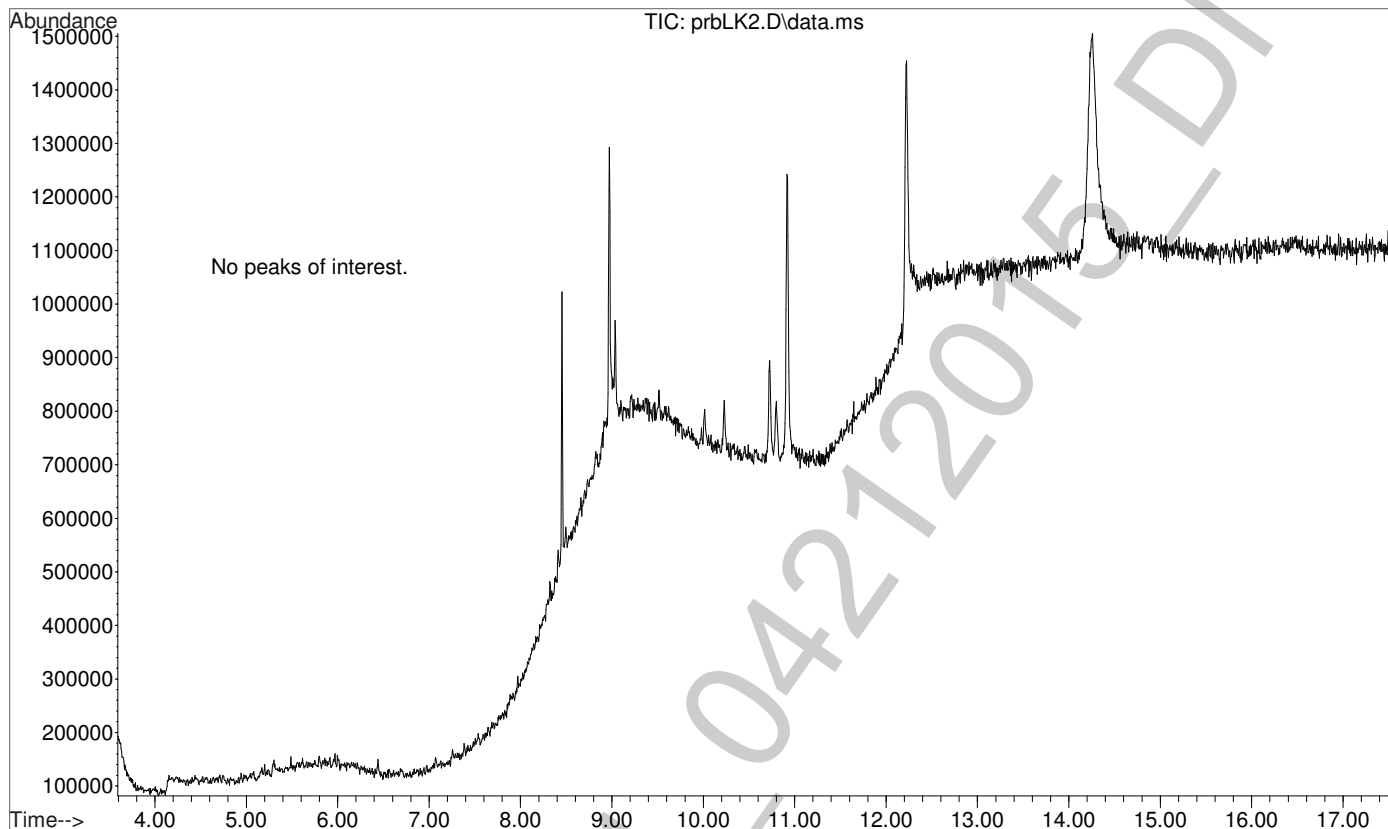

Analytical Method 3.6.1 & 3.6.7 QA Check List

Run Start Date: 04/21/15

Analyst: DND

(Long GC/MS temperature program)

Positive Control Compound List



- Methamphetamine
- Nicotine
- Meperidine
- Caffeine
- Diphenhydramine
- Lidocaine
- PCP
- Methadone
- Amitriptyline
- Codeine
- Trazodone

Internal Standards


- Benzphetamine
- Papaverine

Optional back extraction **not** performed.
Samples reconstituted in methanol.



File :C:\gcms\1\data\Blood\042115BN\Reinjection Longer GC Method\P
... rerun Solvent Blankr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 21 Apr 2015 12:53 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Pre-run Solvent Blank
Misc Info : Chloroform

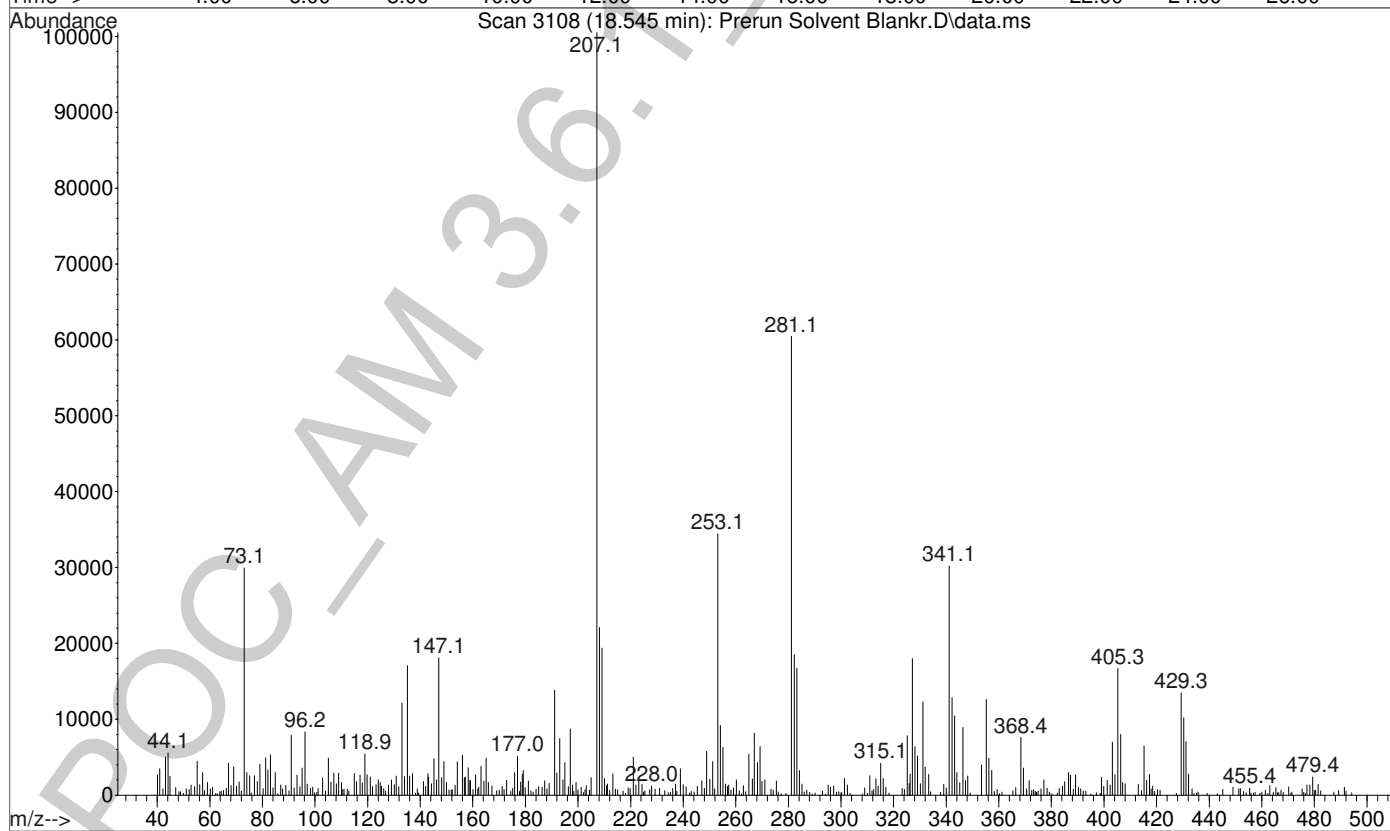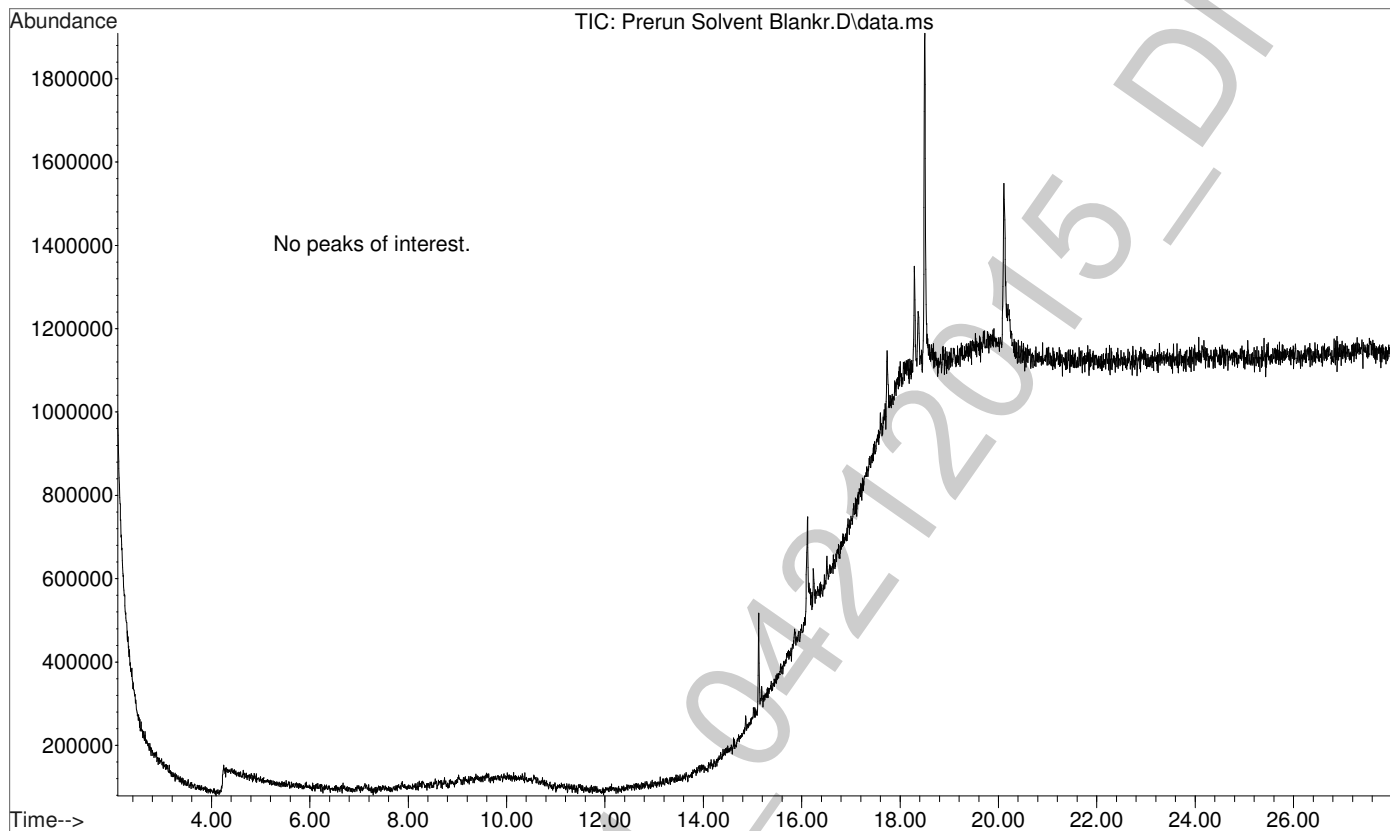



File :C:\gcms\1\data\Blood\042115BN\Reinjection Longer GC Method\N
... egative Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 21 Apr 2015 13:27 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1

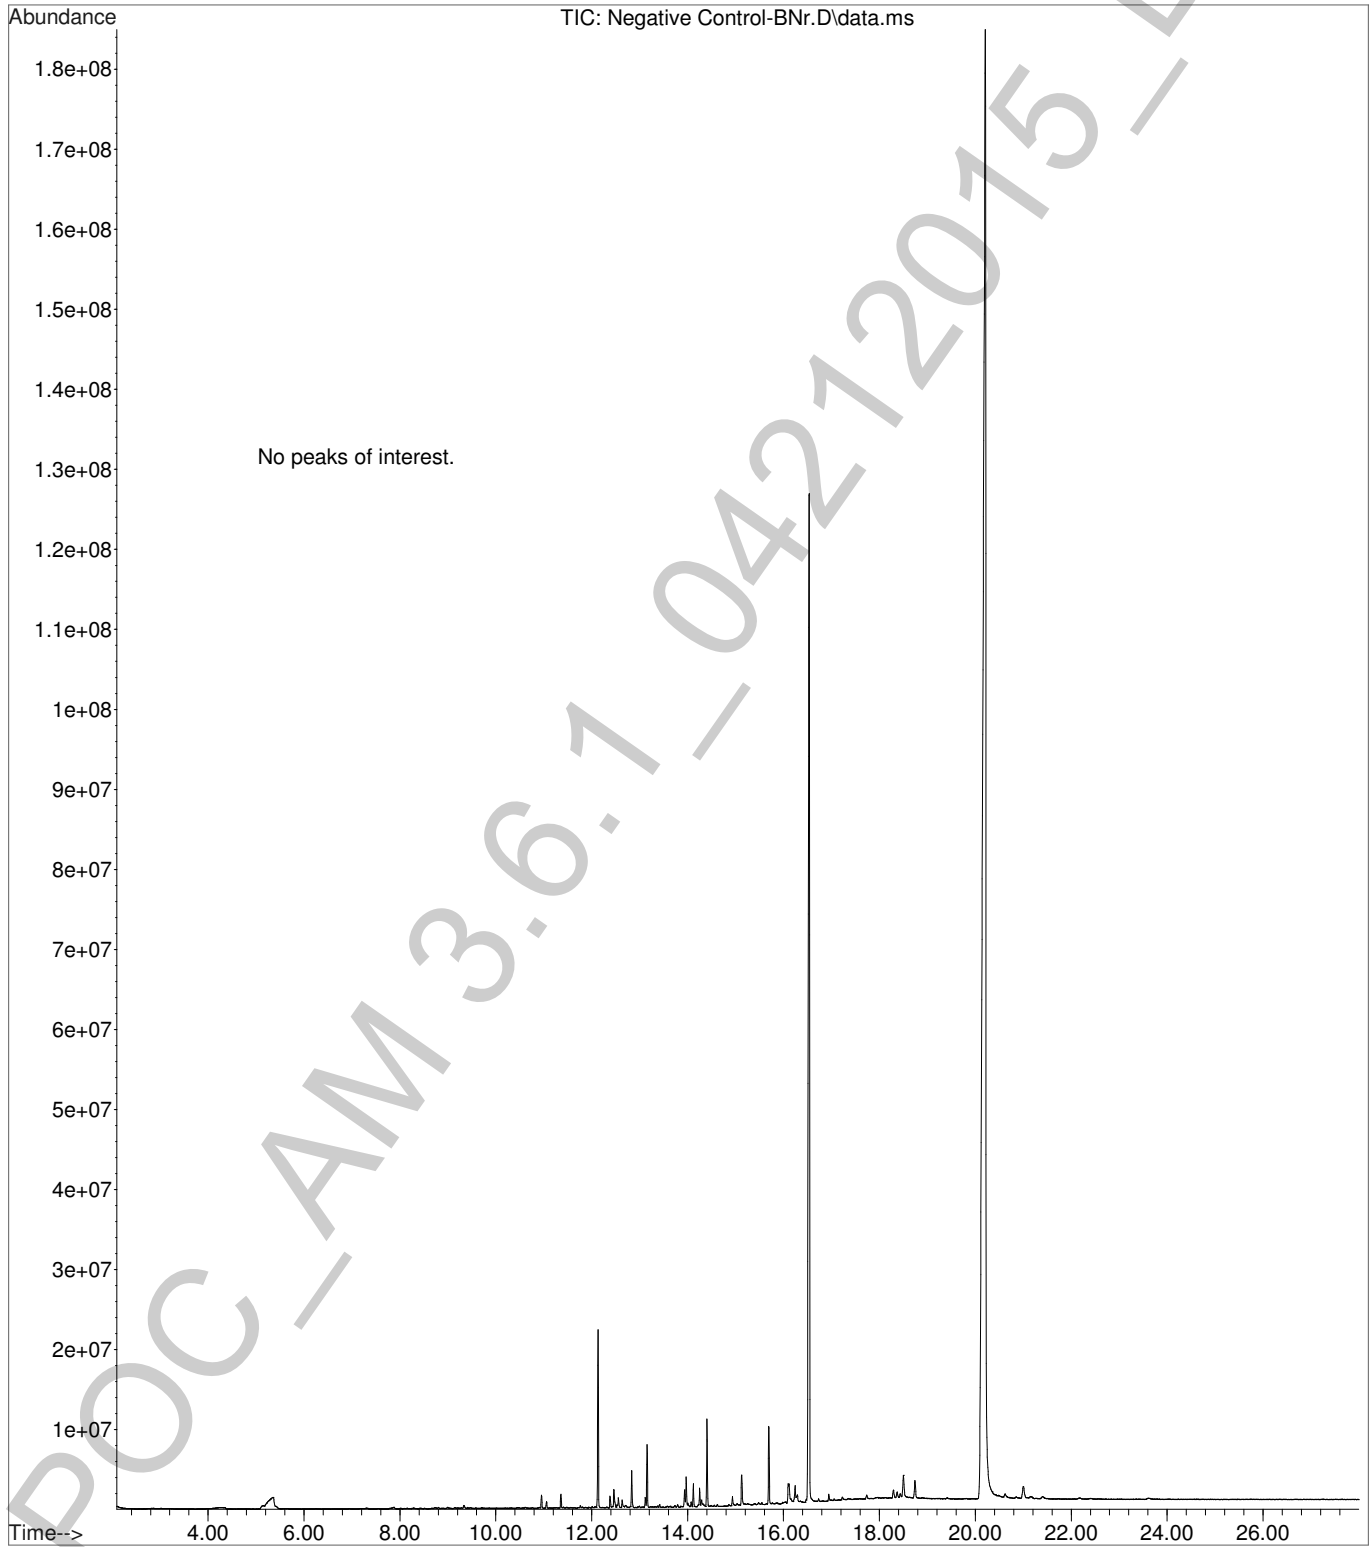


File :C:\gcms\1\data\Blood\042115BN\Reinjection Longer GC Method\N
... egative Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 21 Apr 2015 13:27 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1

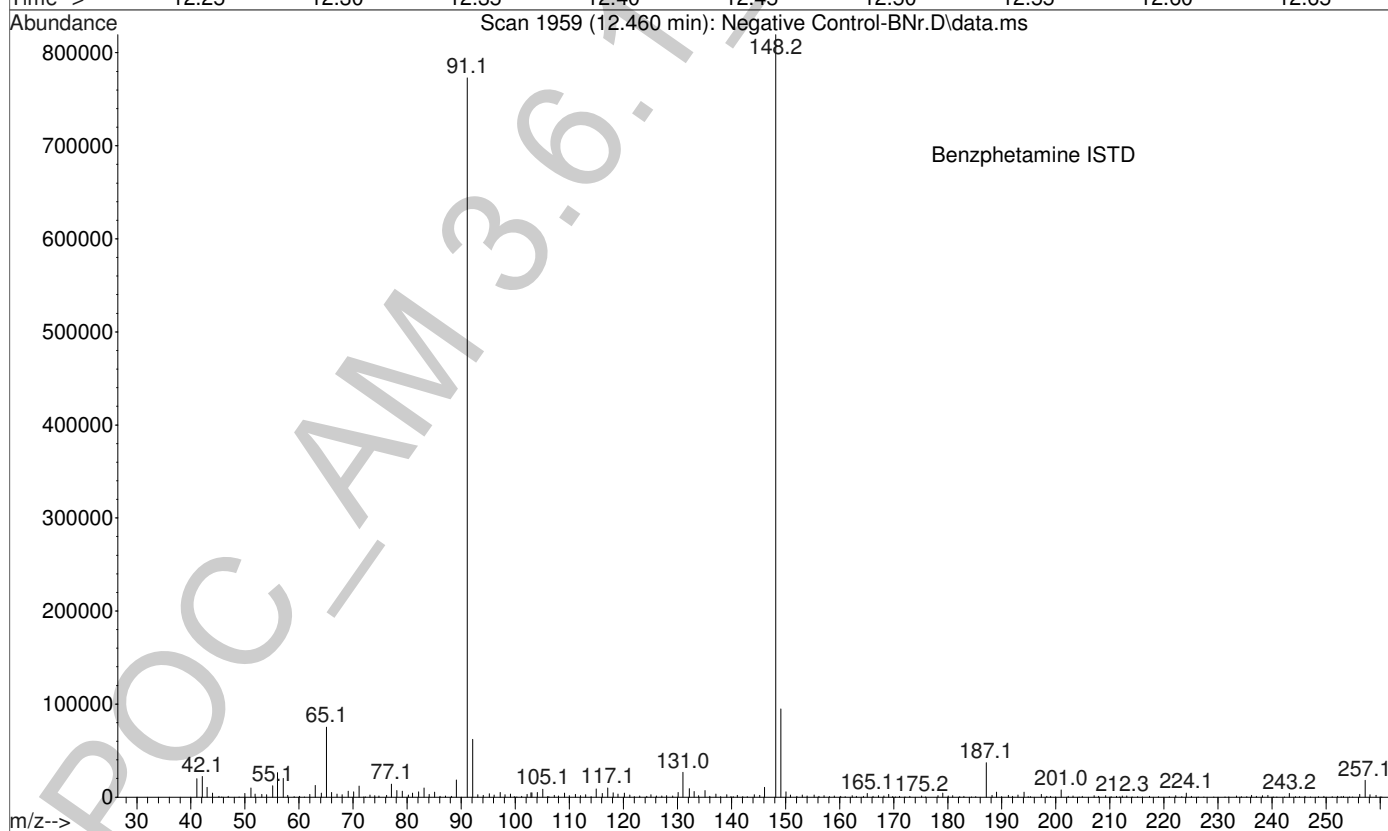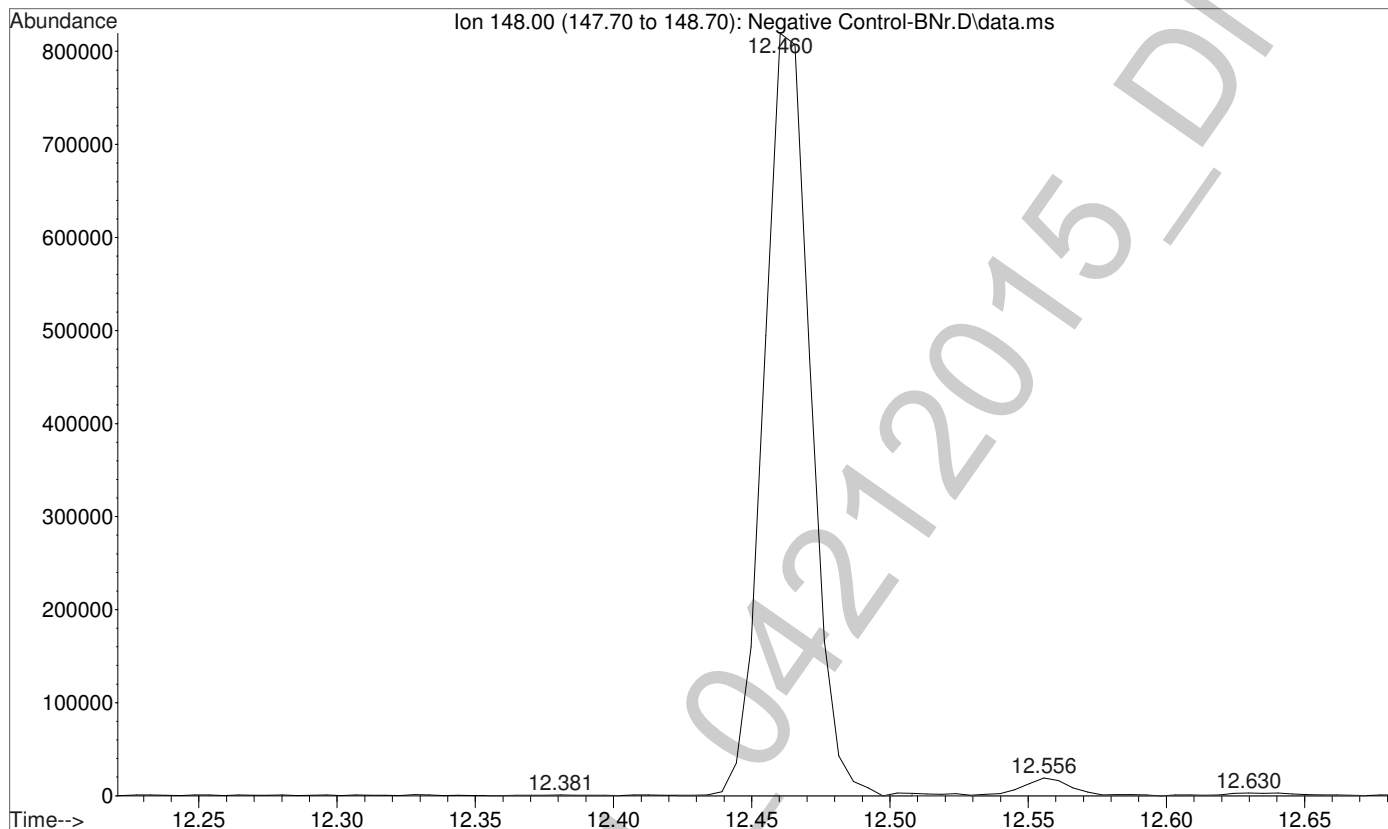



File :C:\gcms\1\data\Blood\042115BN\Reinjection Longer GC Method\N
... egative Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 21 Apr 2015 13:27 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1

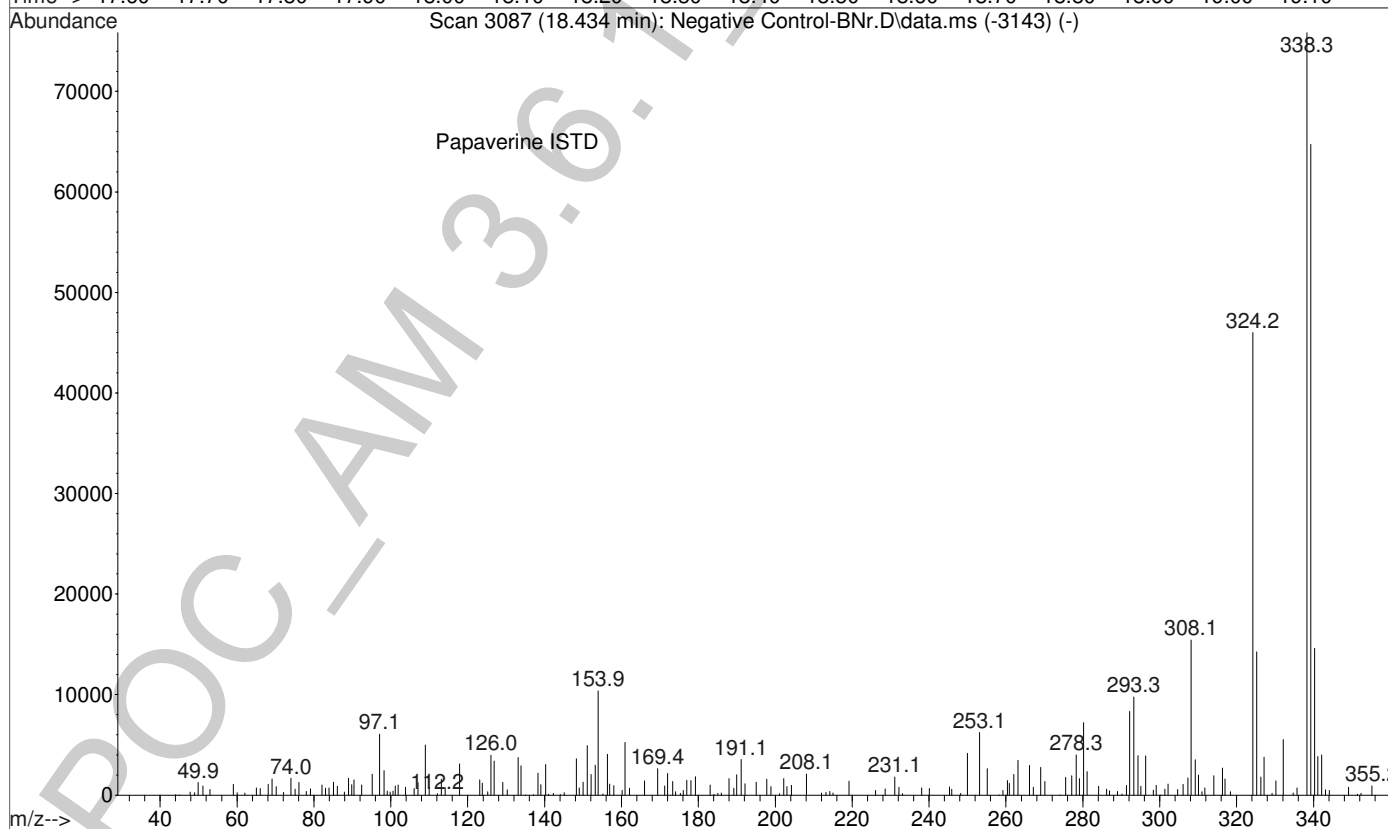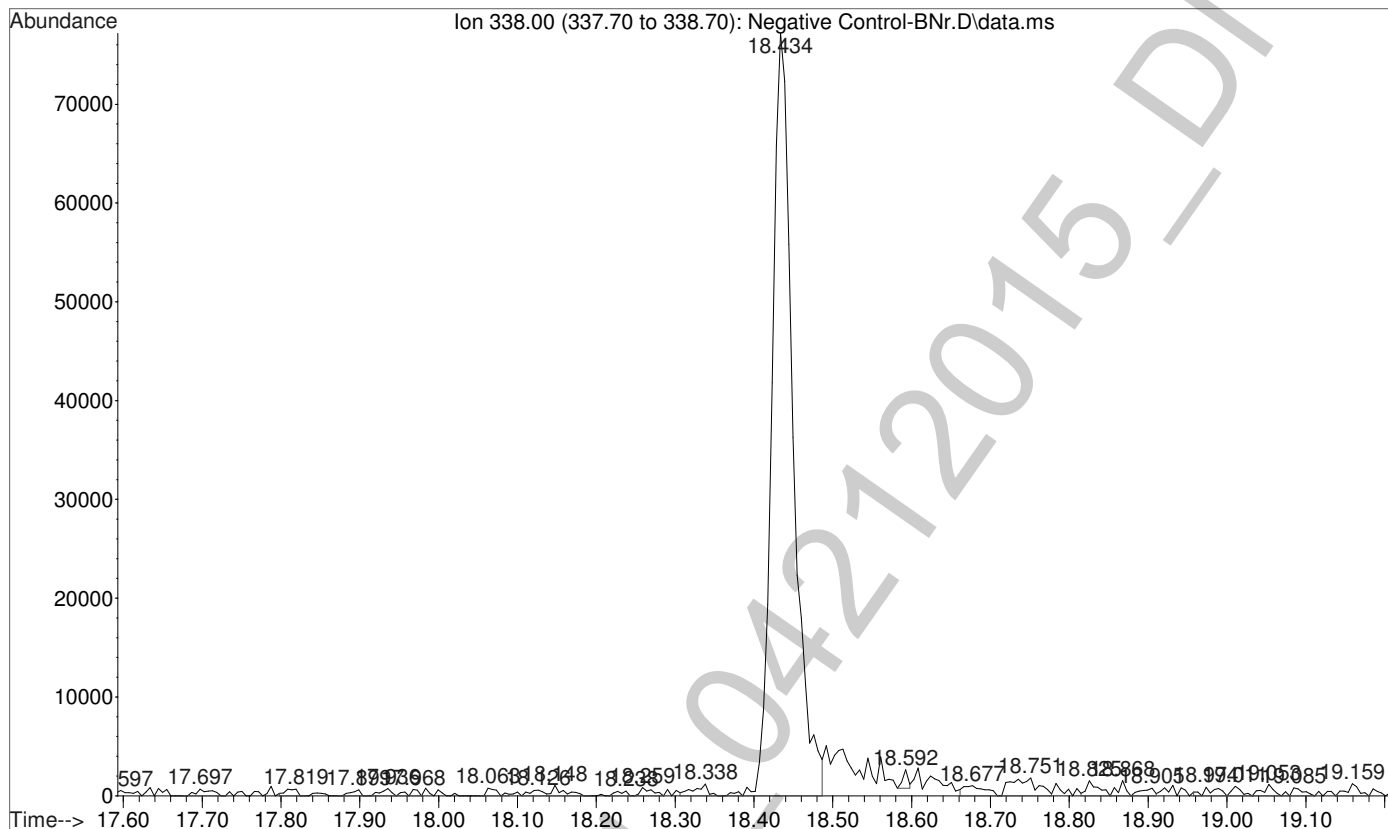



File :C:\gcms\1\data\Blood\042115BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 21 Apr 2015 14:01 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

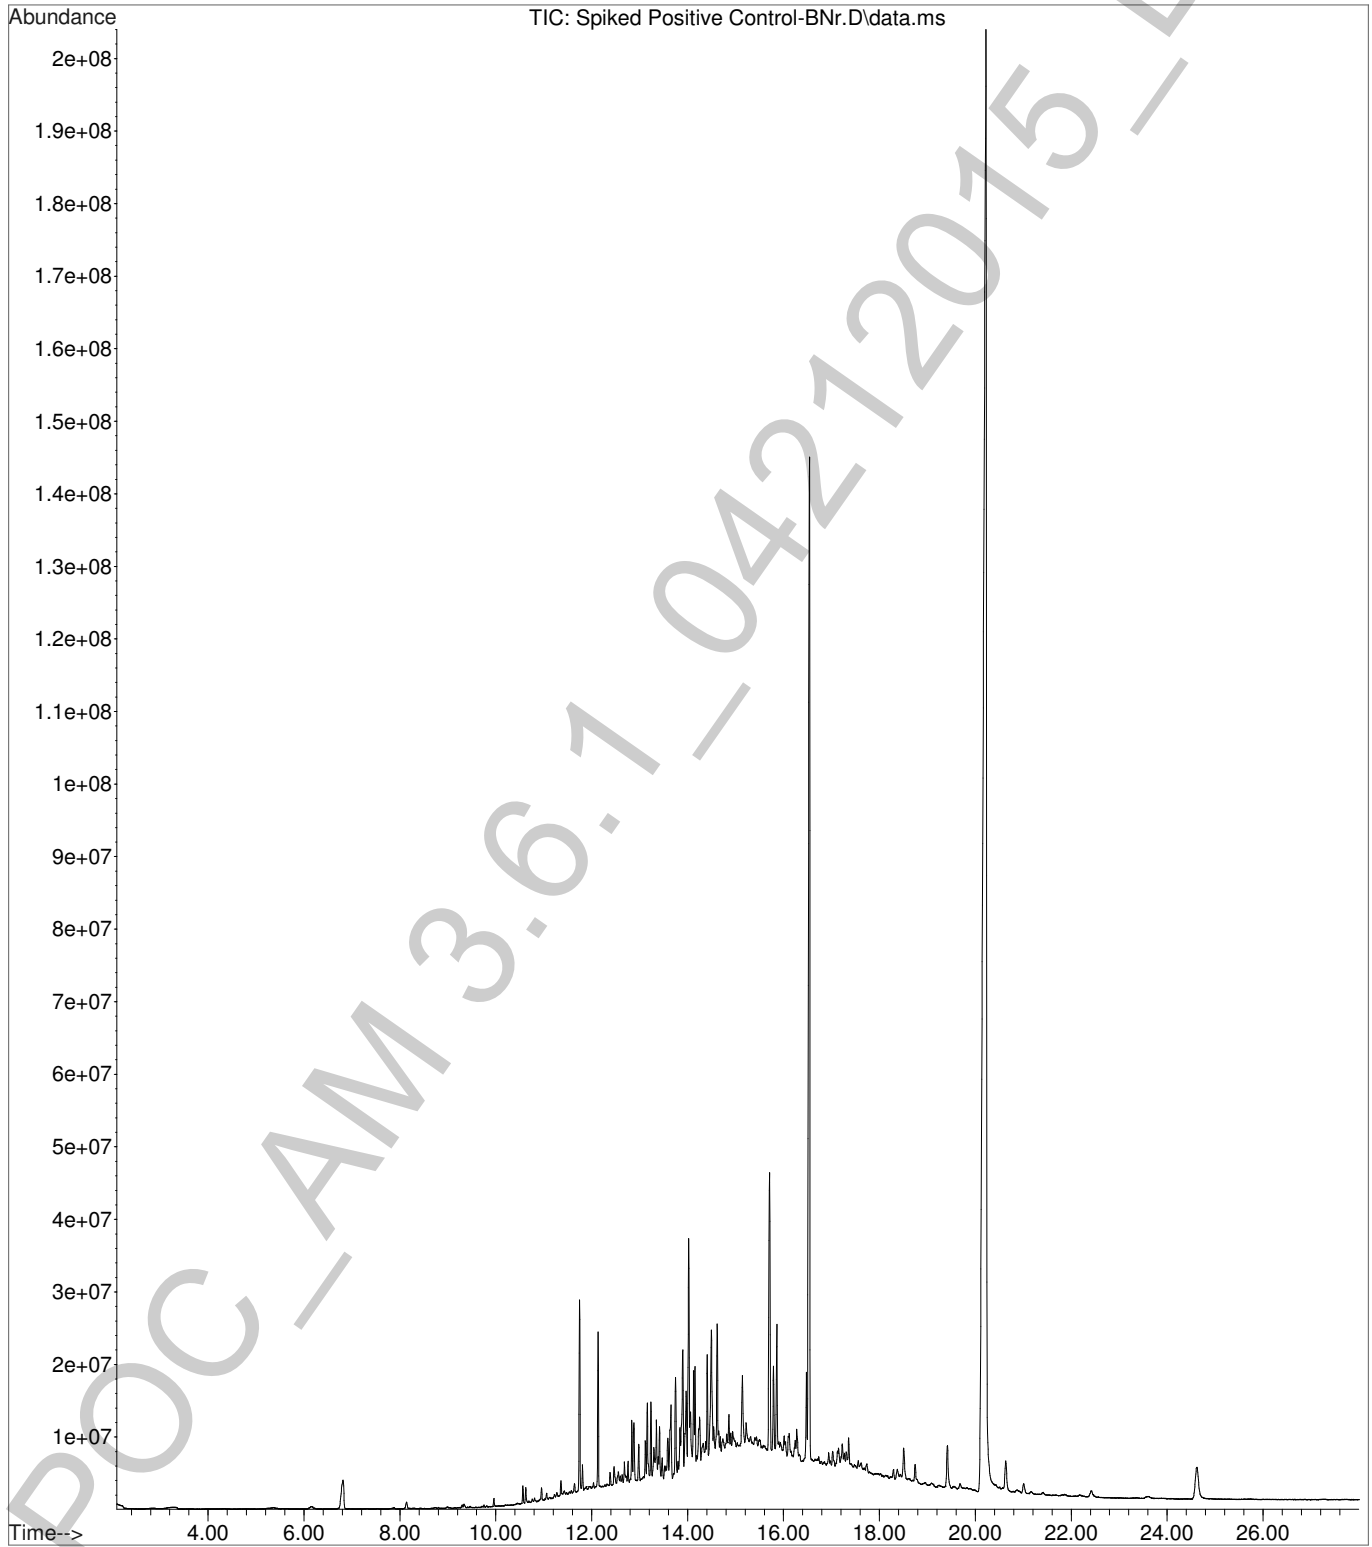



File :C:\gcms\1\data\Blood\042115BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 21 Apr 2015 14:01 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

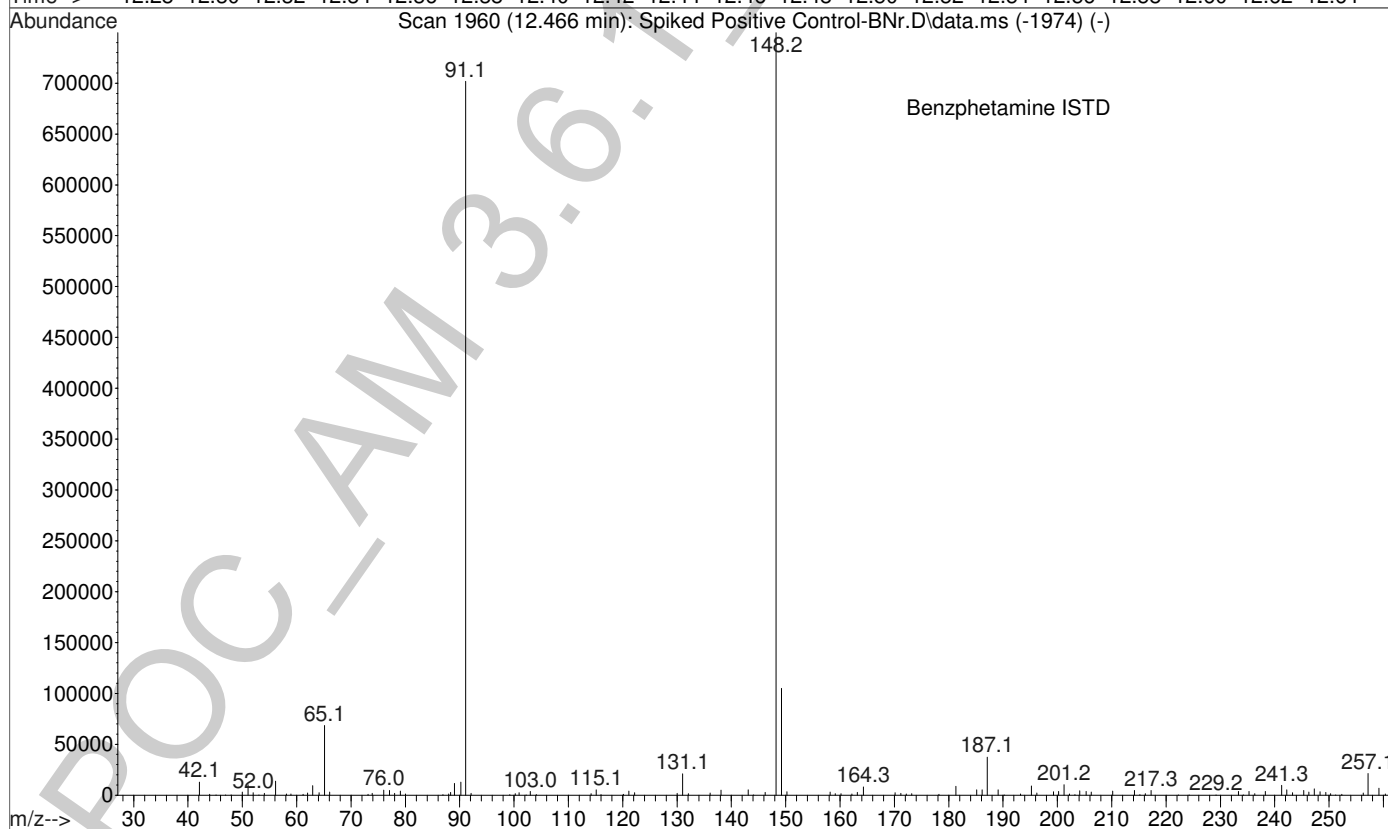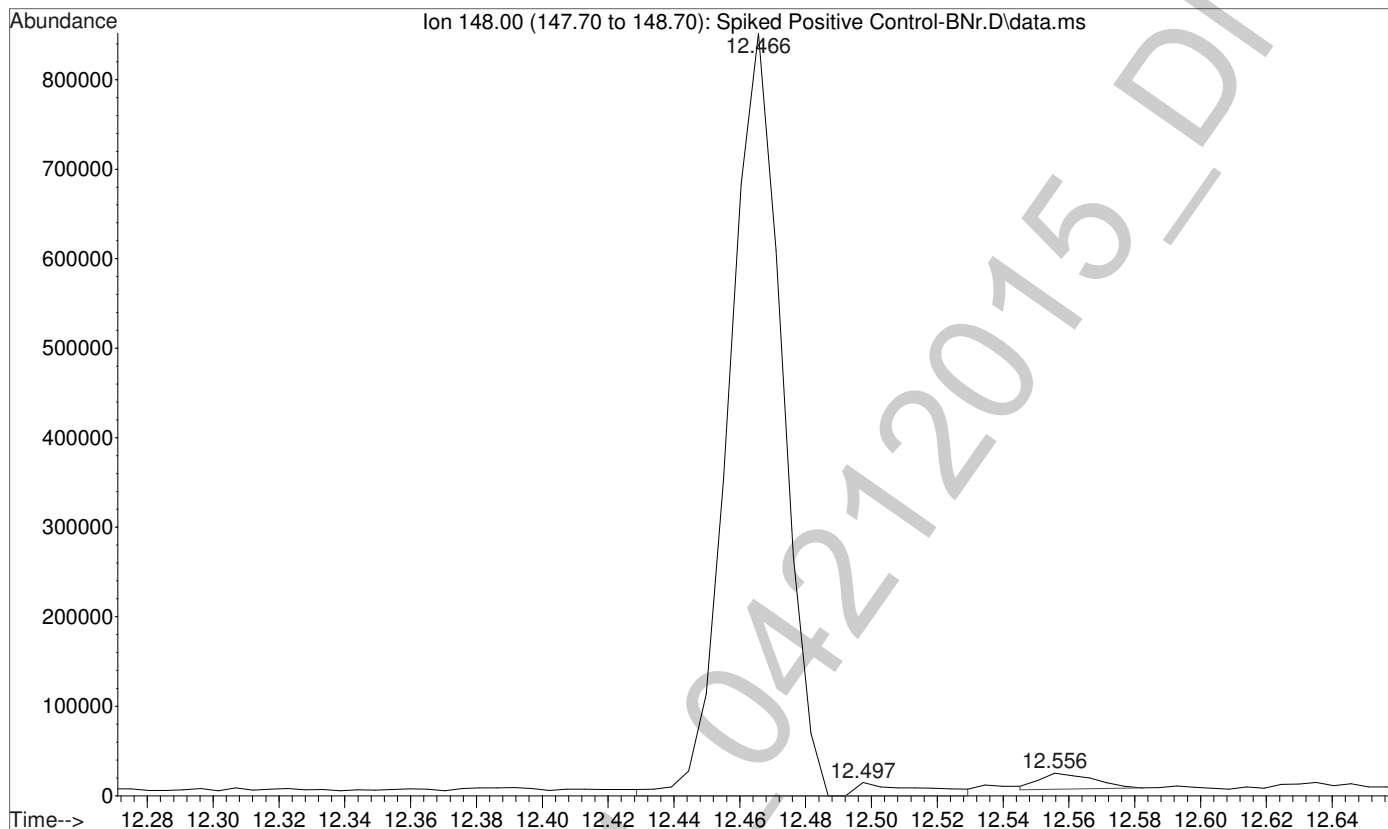



File :C:\gcms\1\data\Blood\042115BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 21 Apr 2015 14:01 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

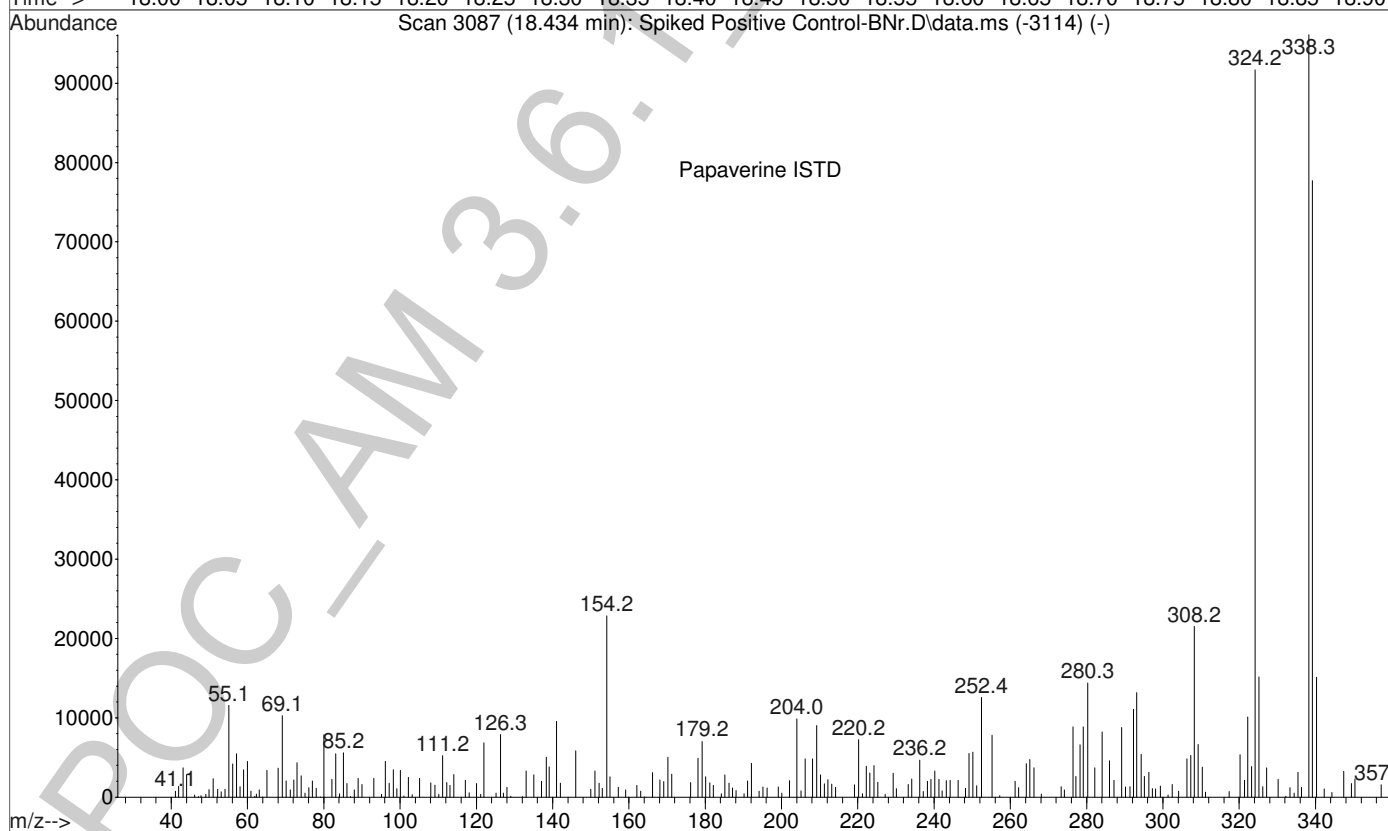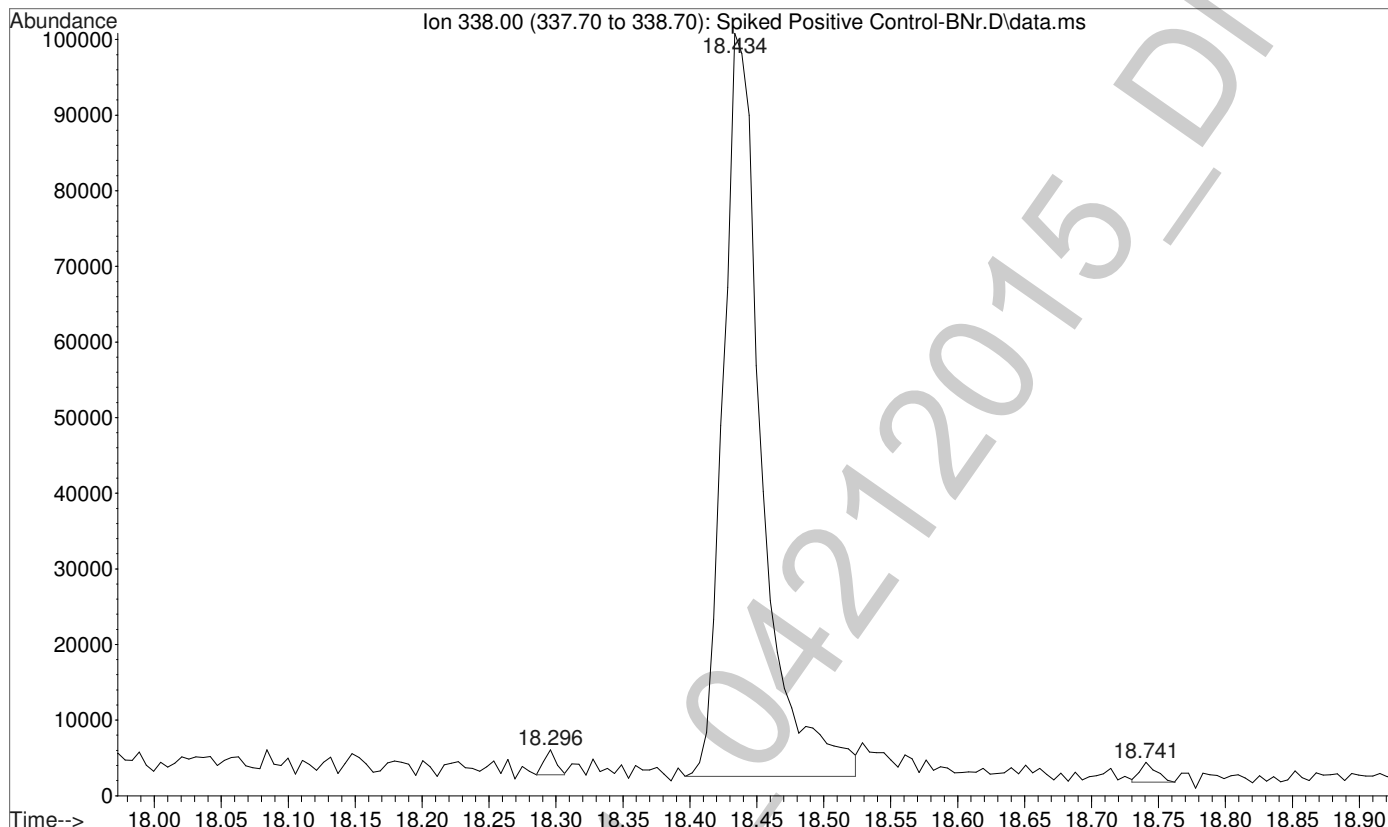



File :C:\gcms\1\data\Blood\042115BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 21 Apr 2015 14:01 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

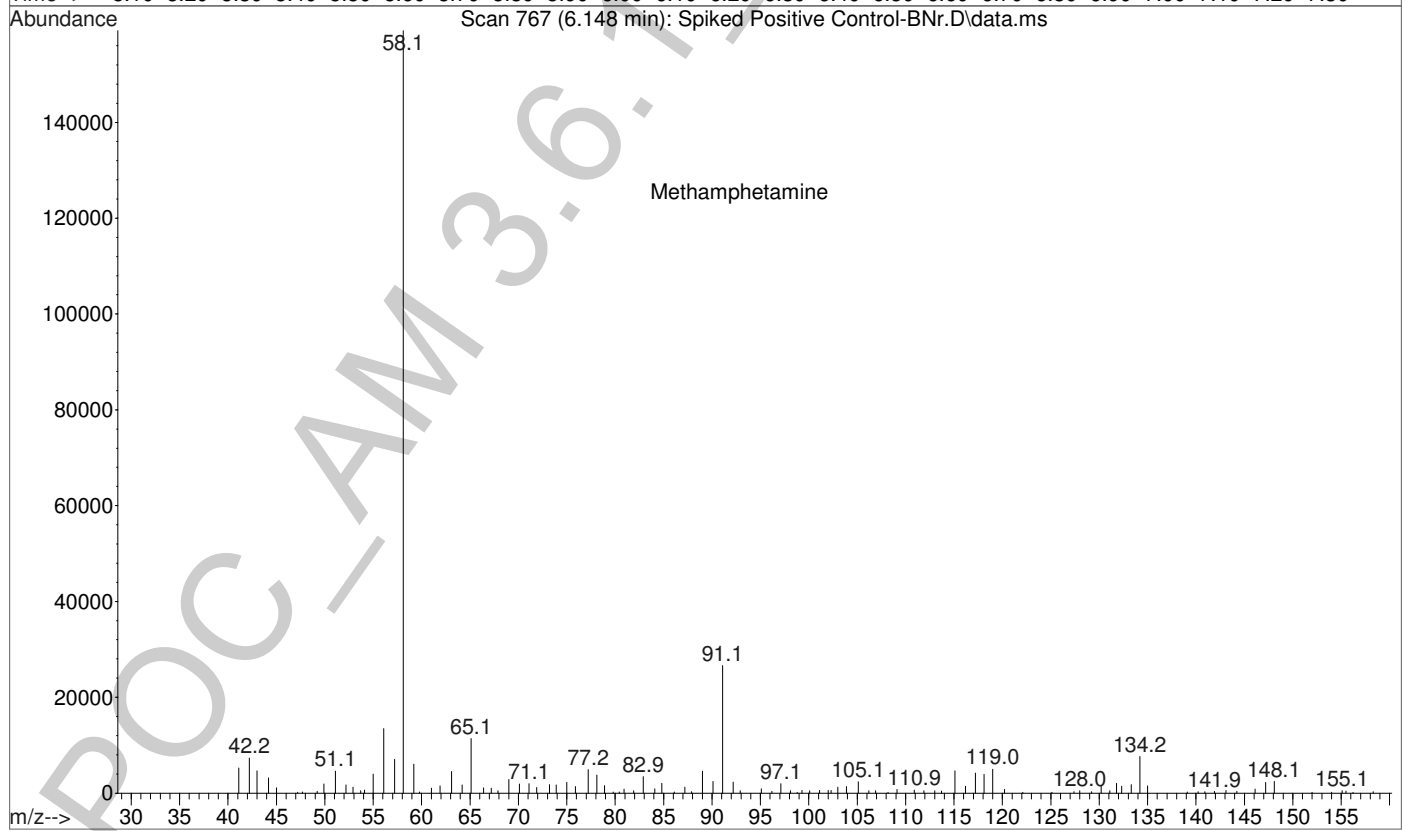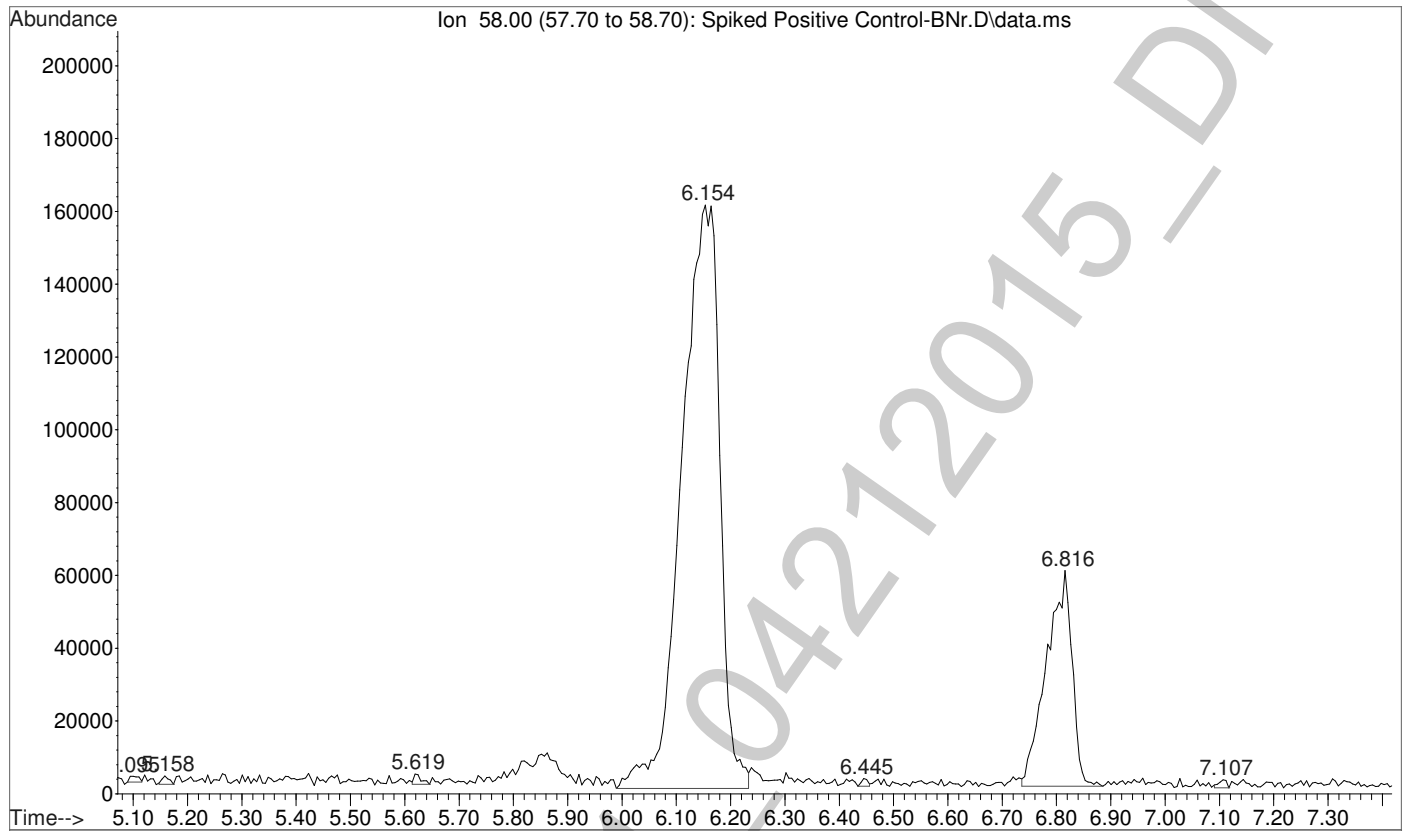



File :C:\gcms\1\data\Blood\042115BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 21 Apr 2015 14:01 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

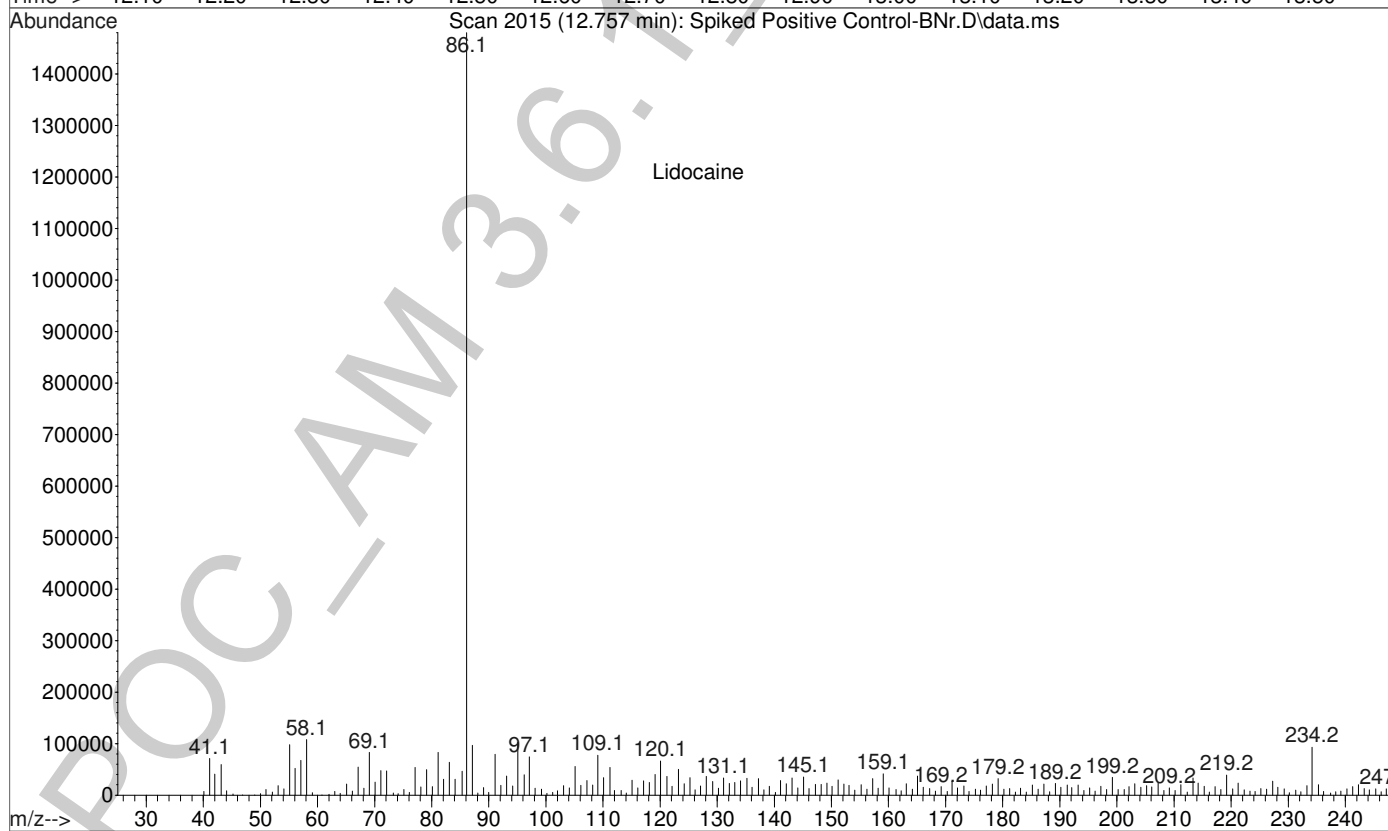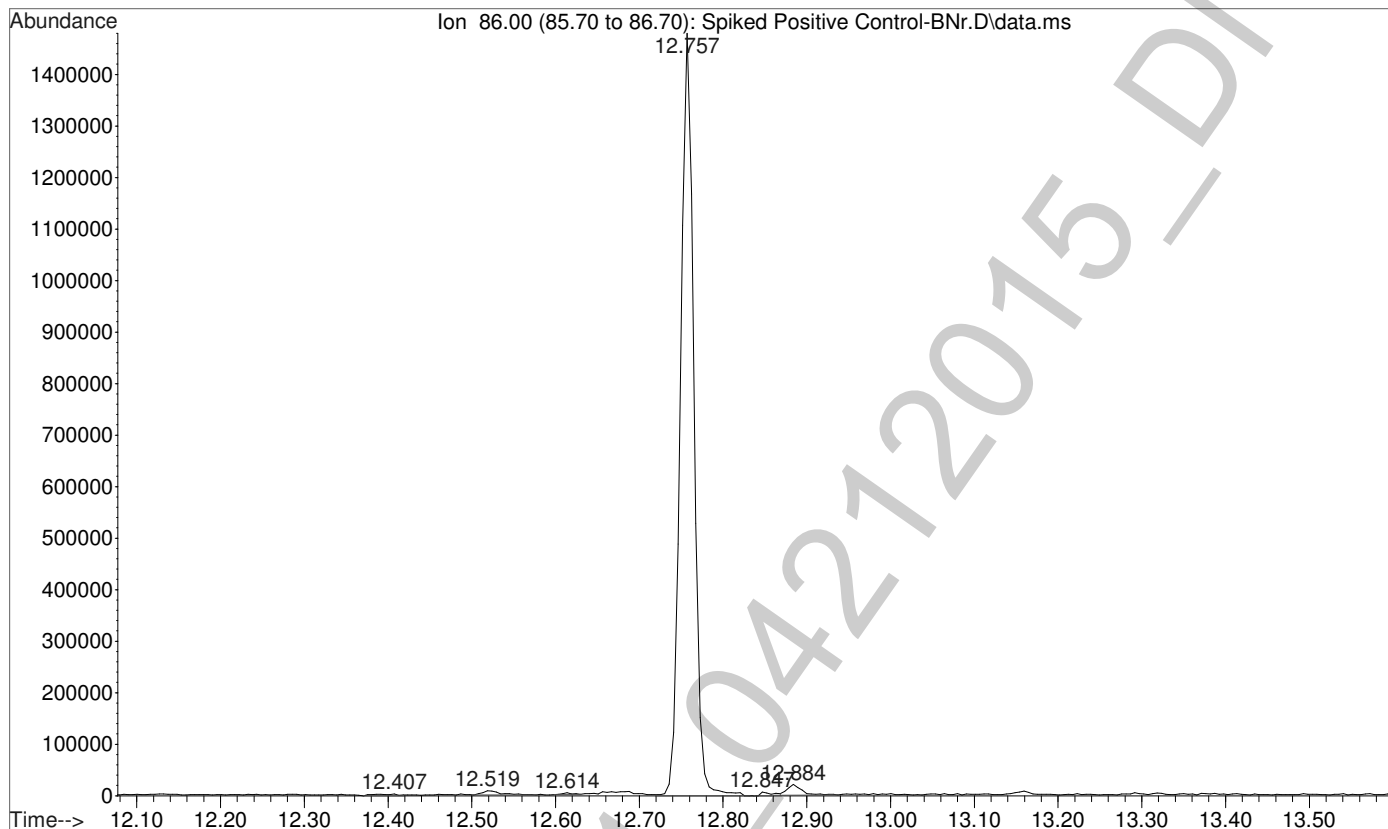



File :C:\gcms\1\data\Blood\042115BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 21 Apr 2015 14:01 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

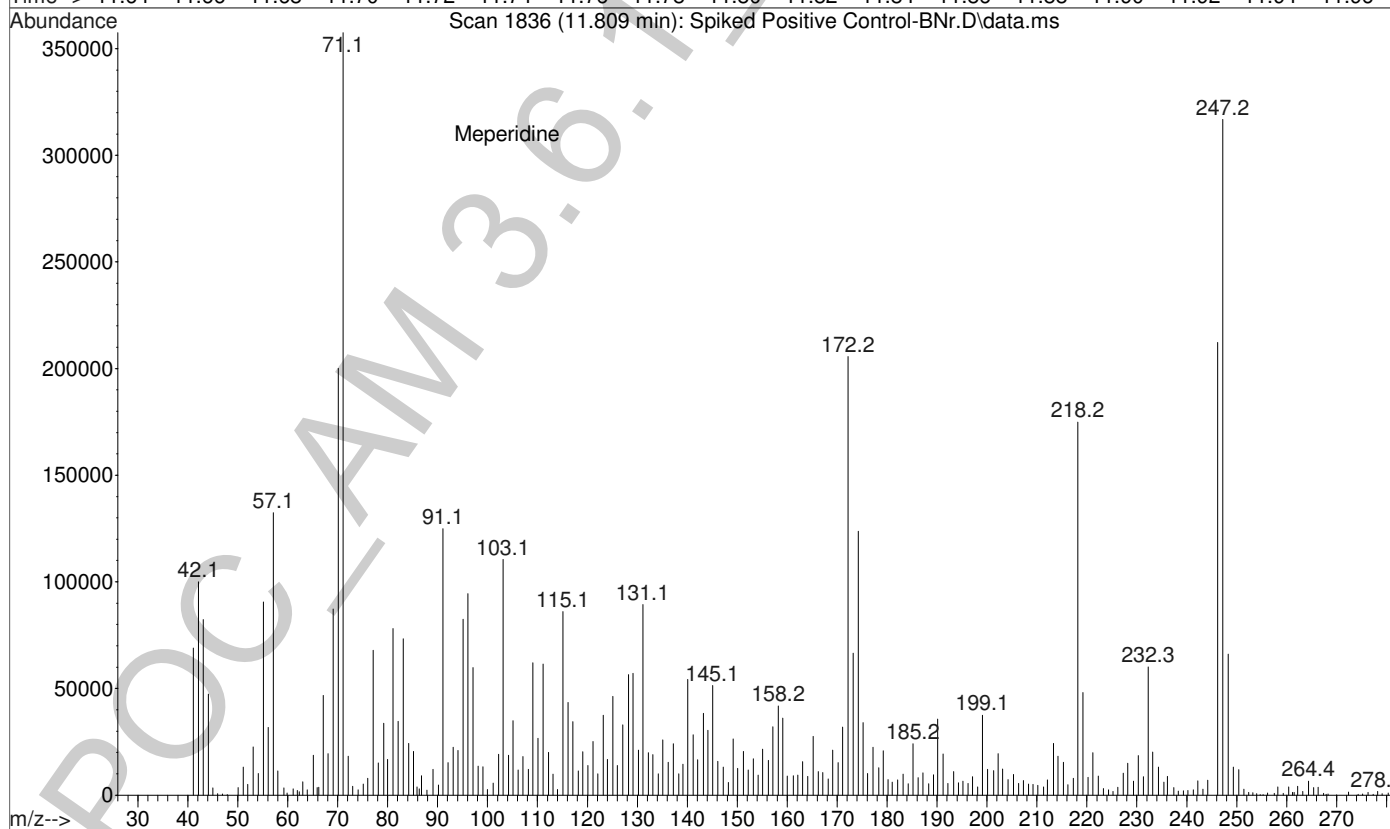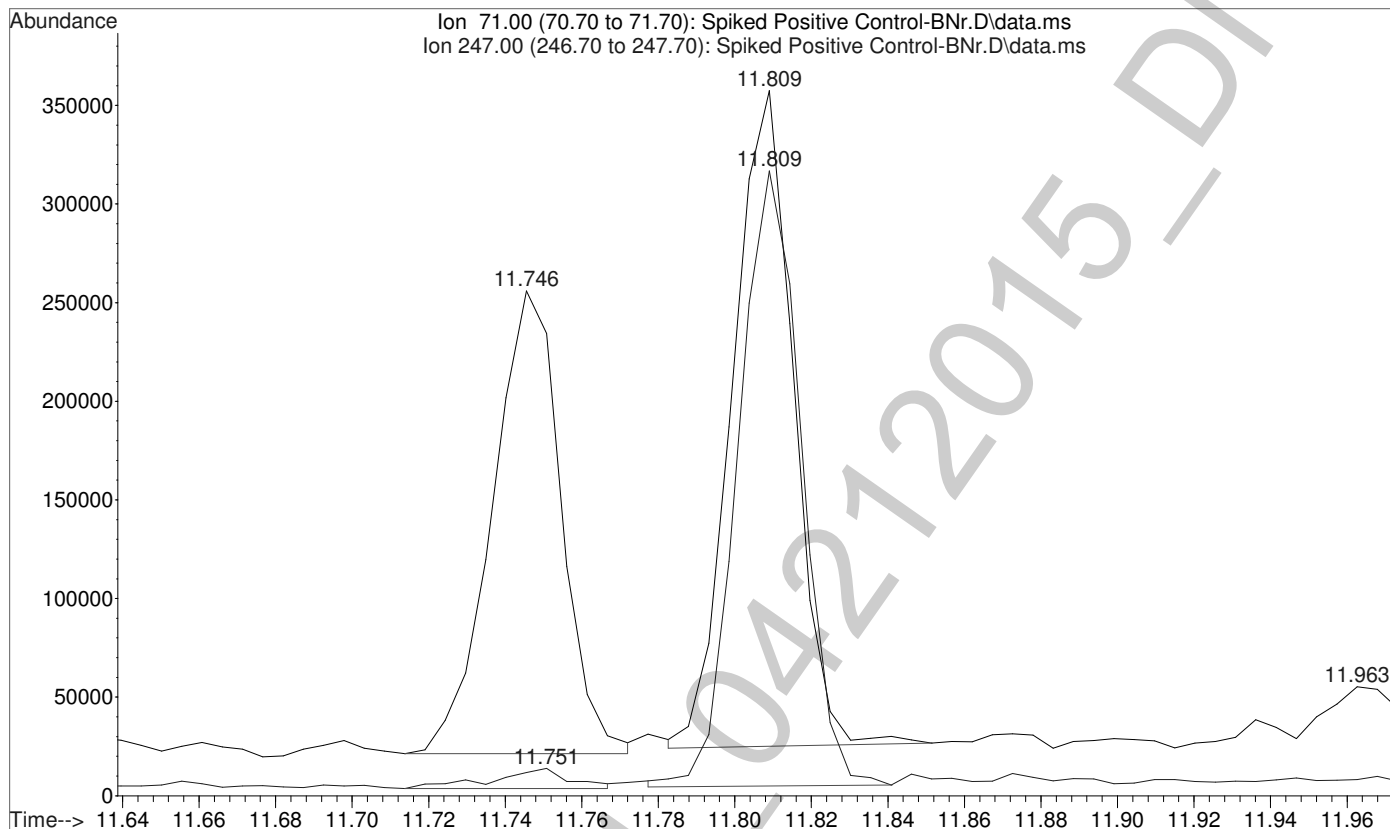



File :C:\gcms\1\data\Blood\042115BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 21 Apr 2015 14:01 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

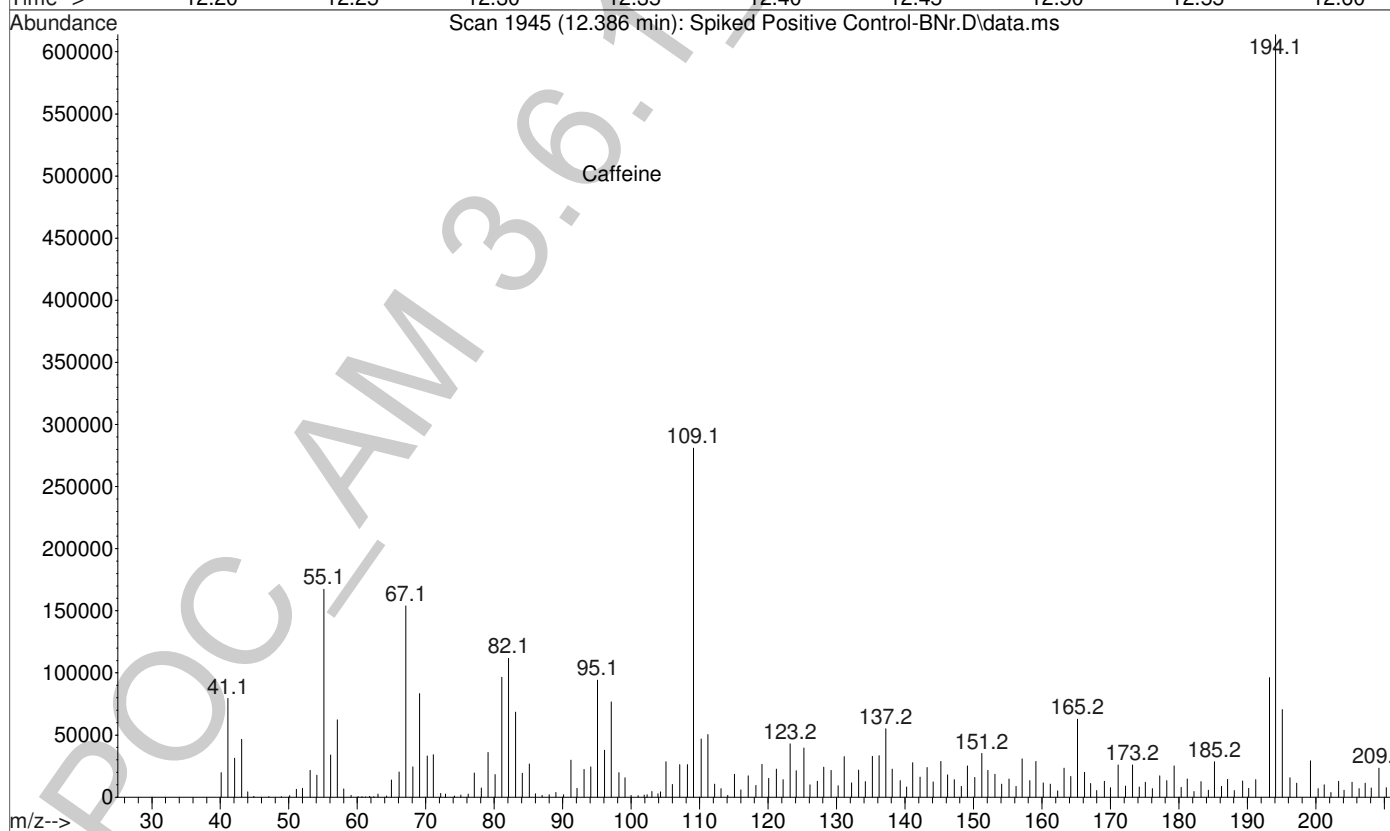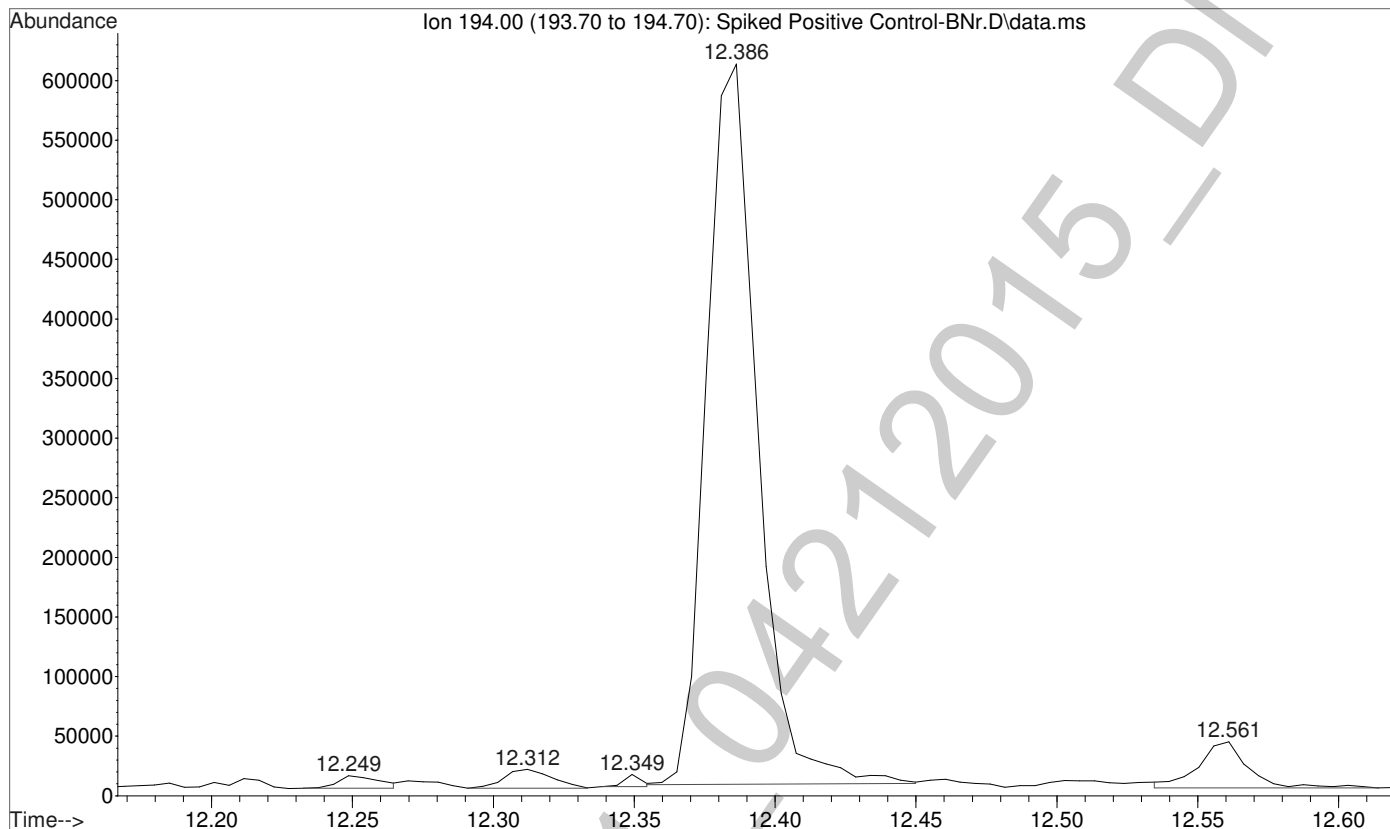



File :C:\gcms\1\data\Blood\042115BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 21 Apr 2015 14:01 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

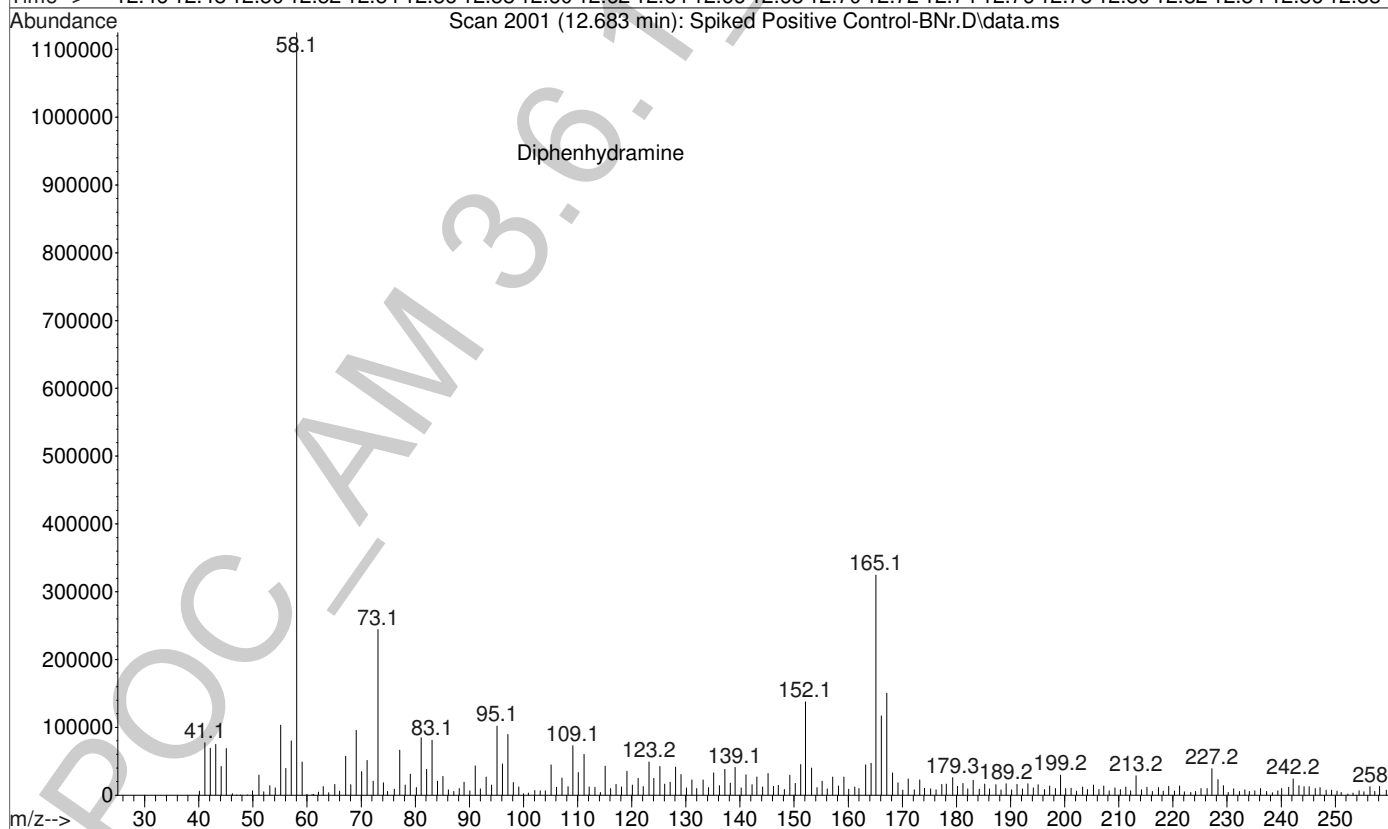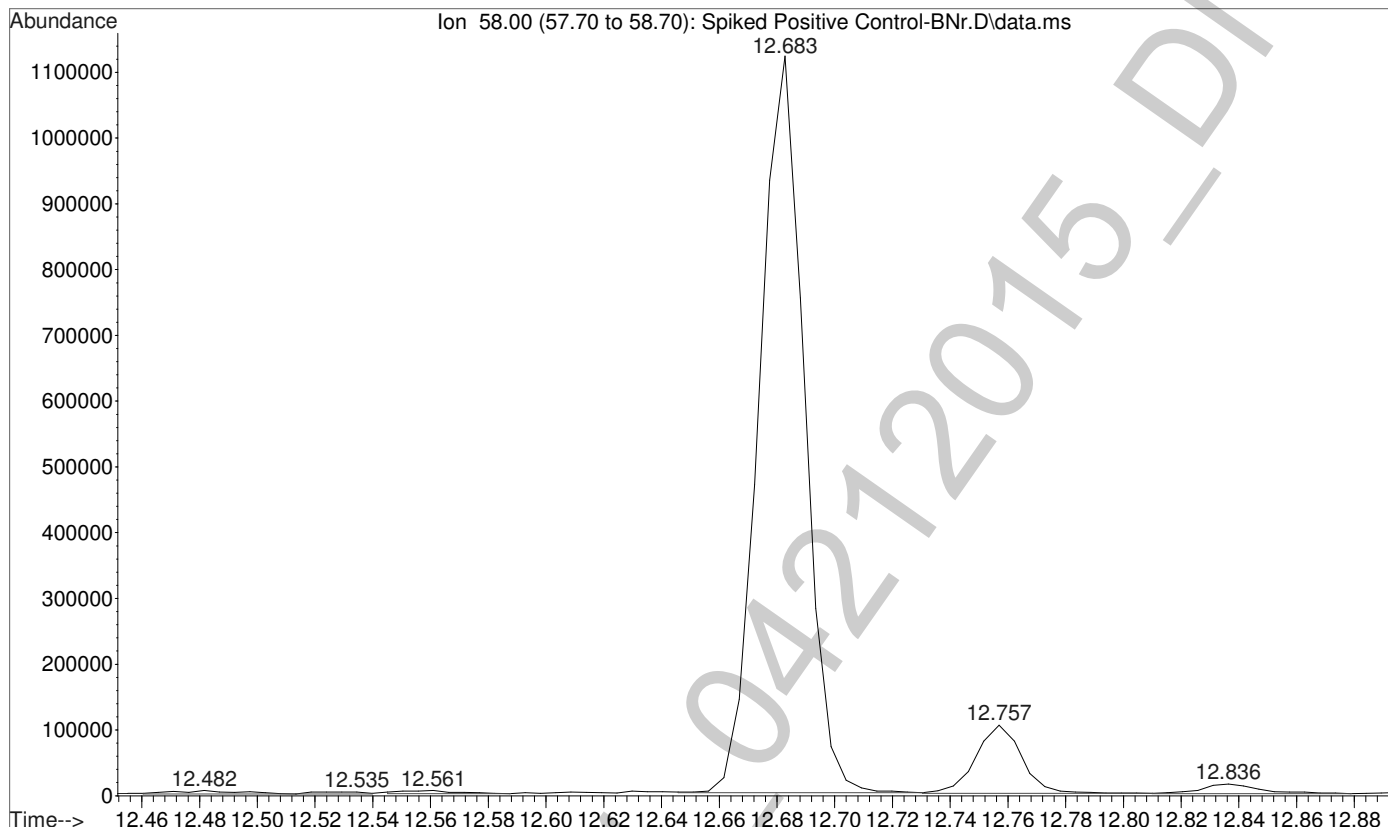



File :C:\gcms\1\data\Blood\042115BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 21 Apr 2015 14:01 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

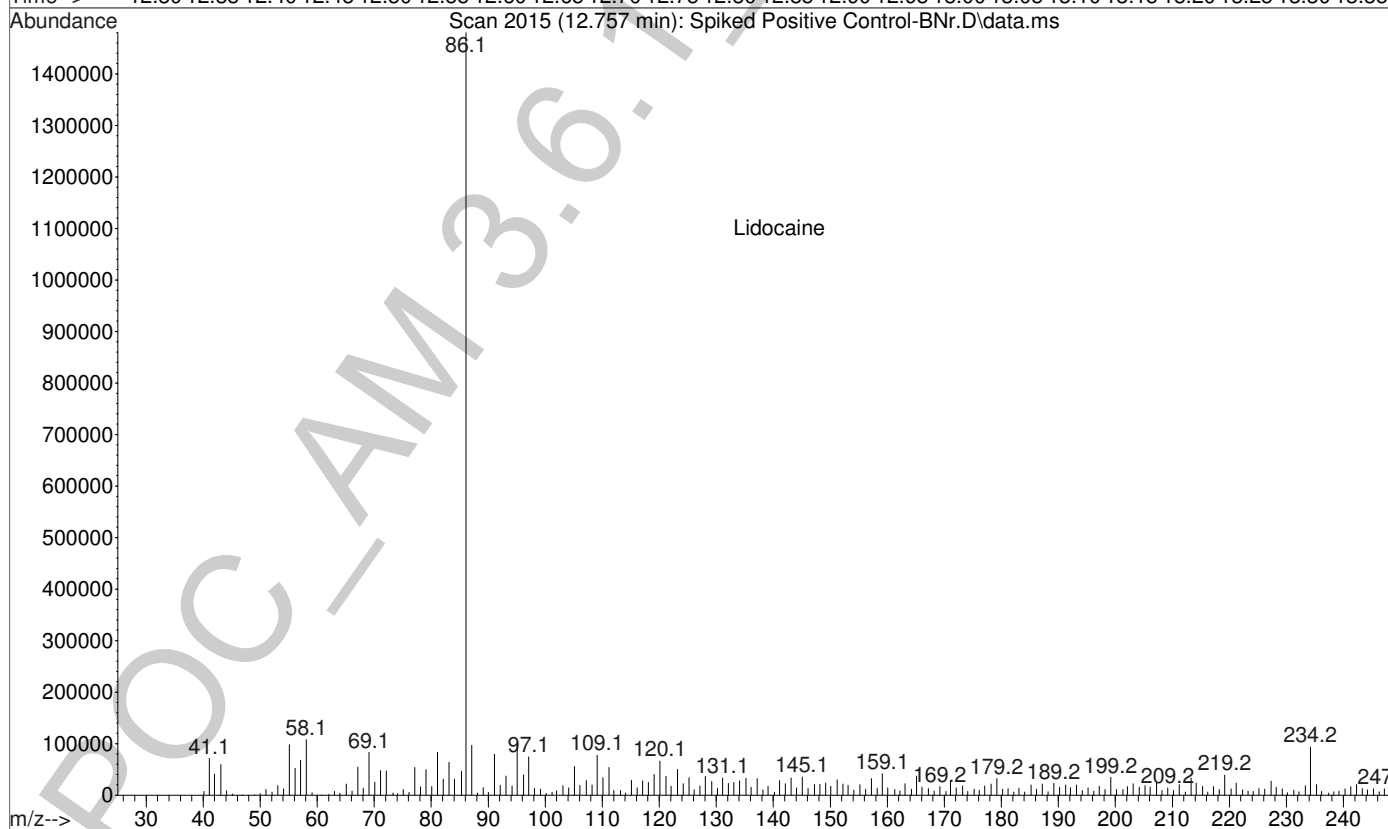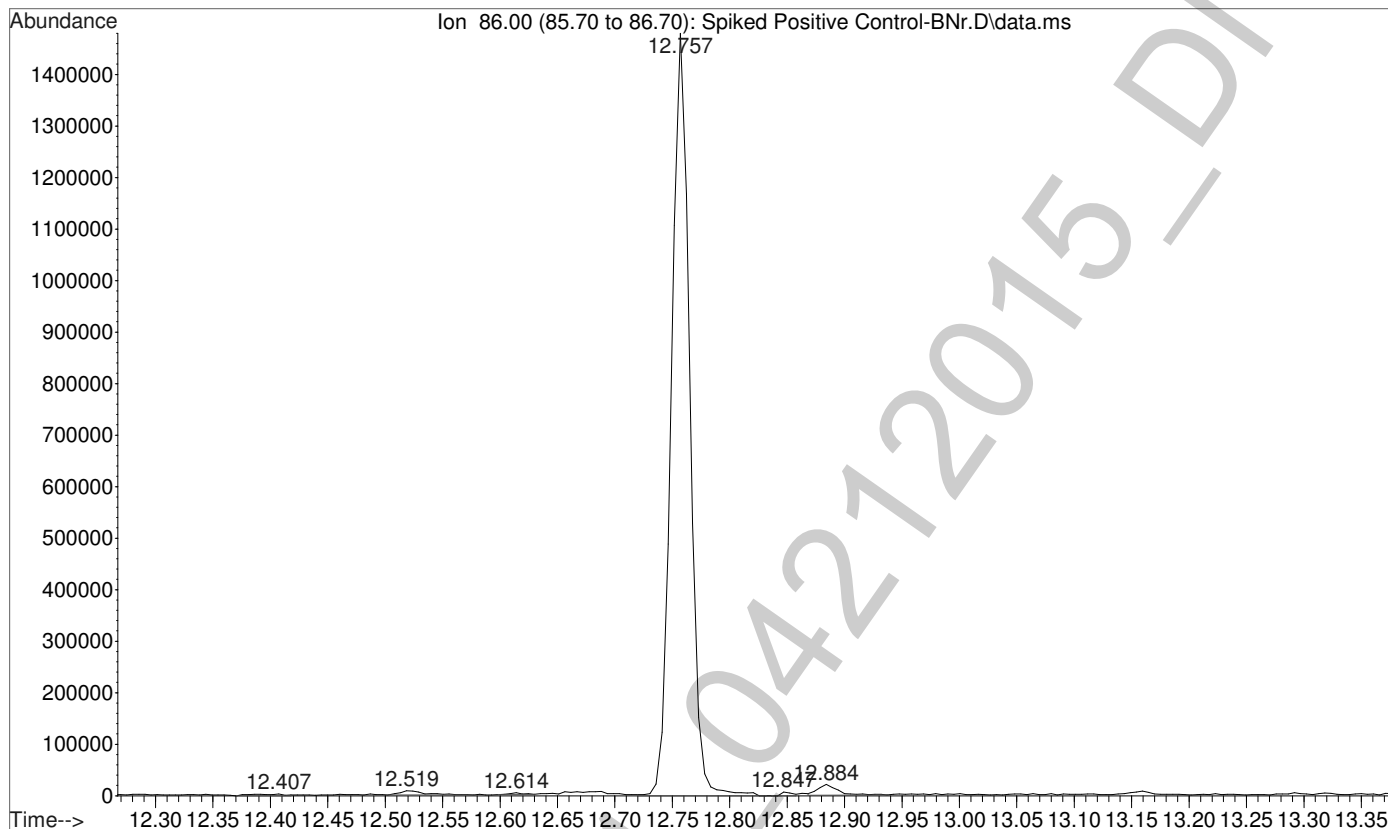



File :C:\gcms\1\data\Blood\042115BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 21 Apr 2015 14:01 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

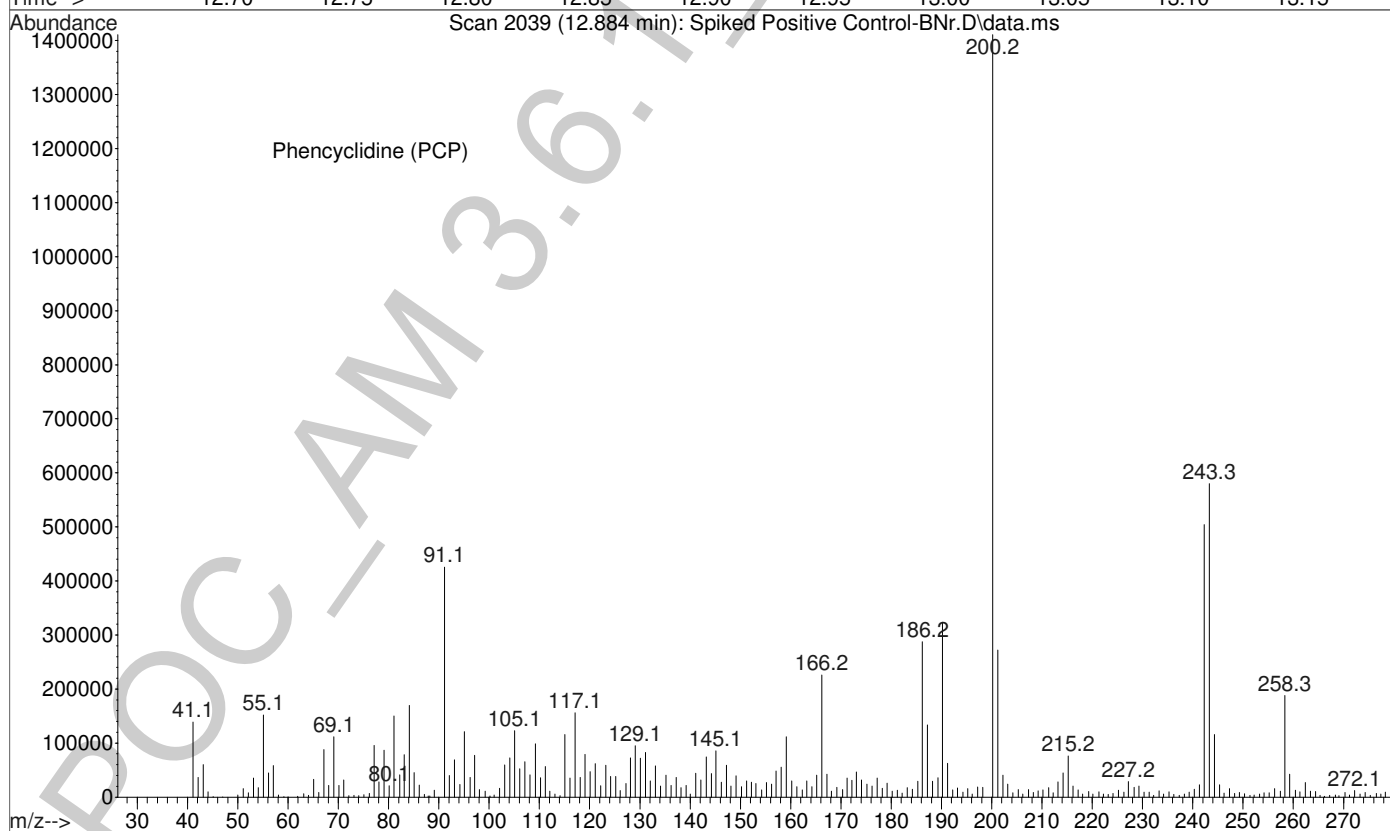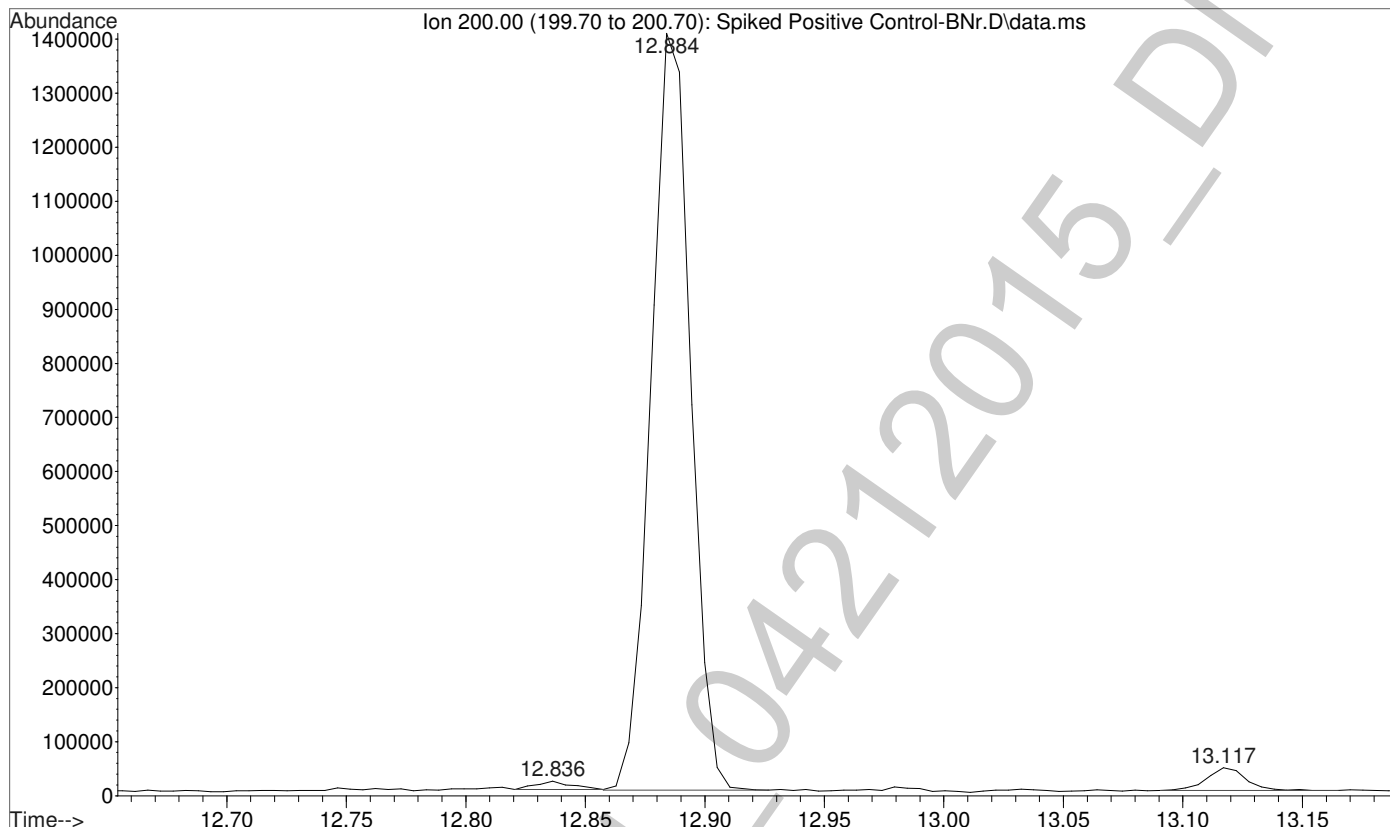



File :C:\gcms\1\data\Blood\042115BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 21 Apr 2015 14:01 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

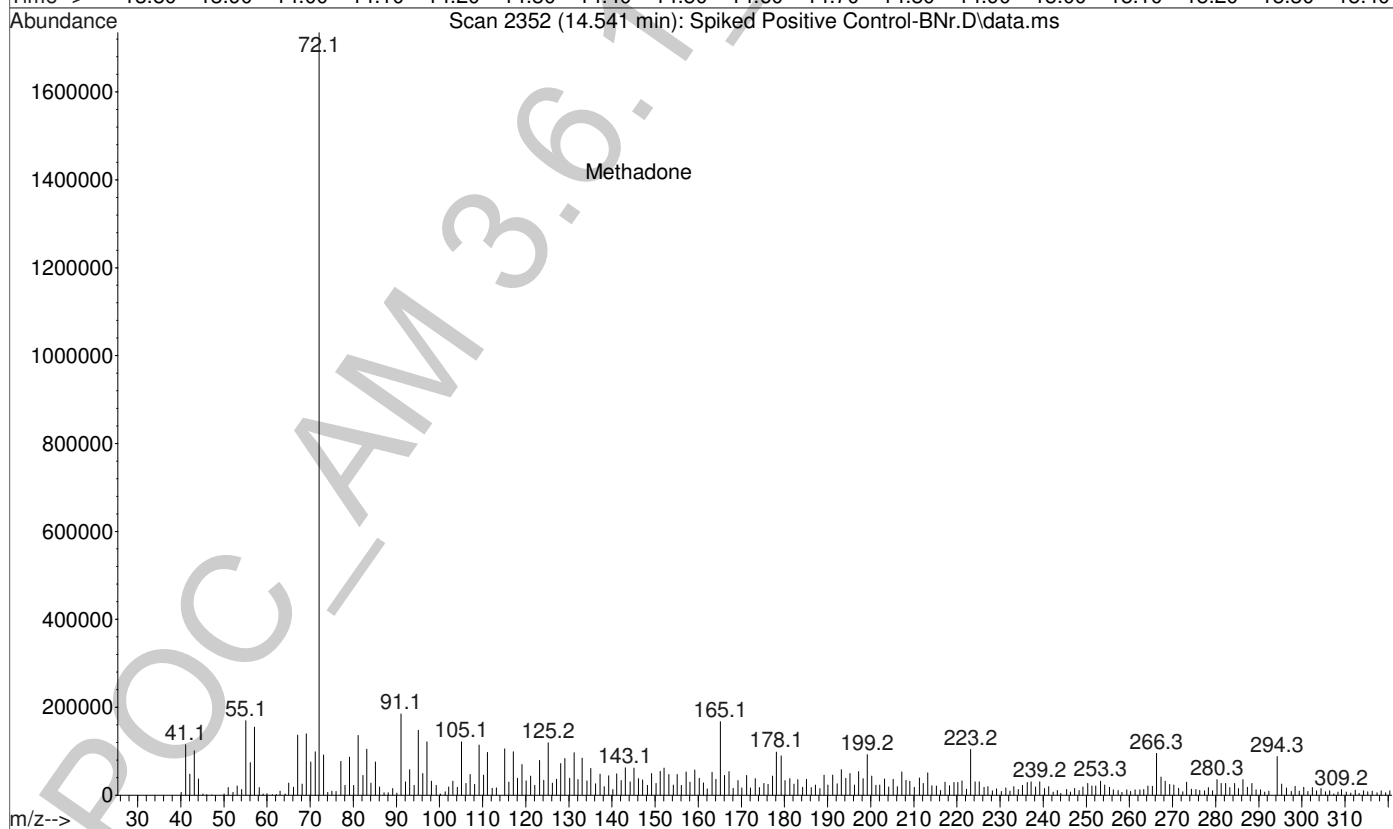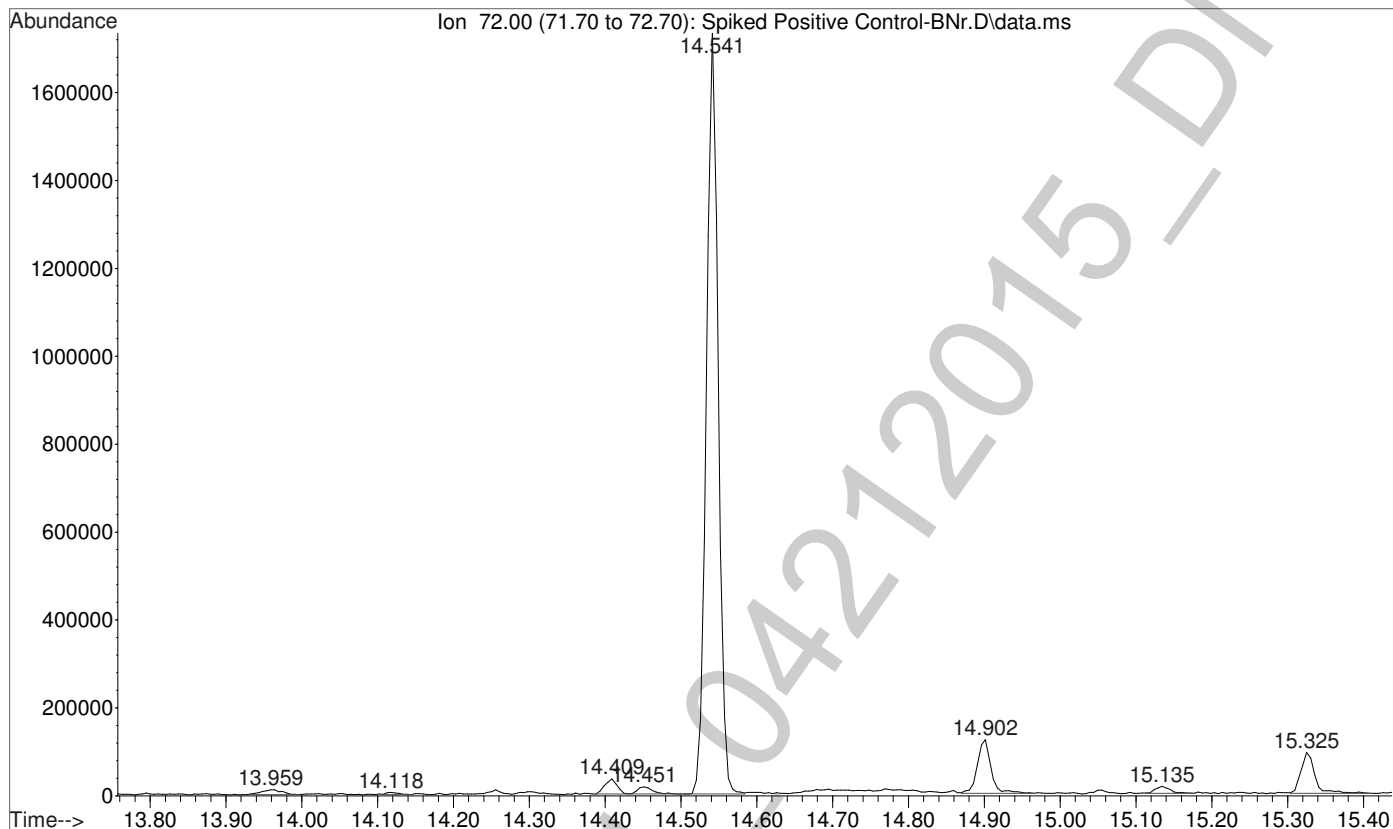



File :C:\gcms\1\data\Blood\042115BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 21 Apr 2015 14:01 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

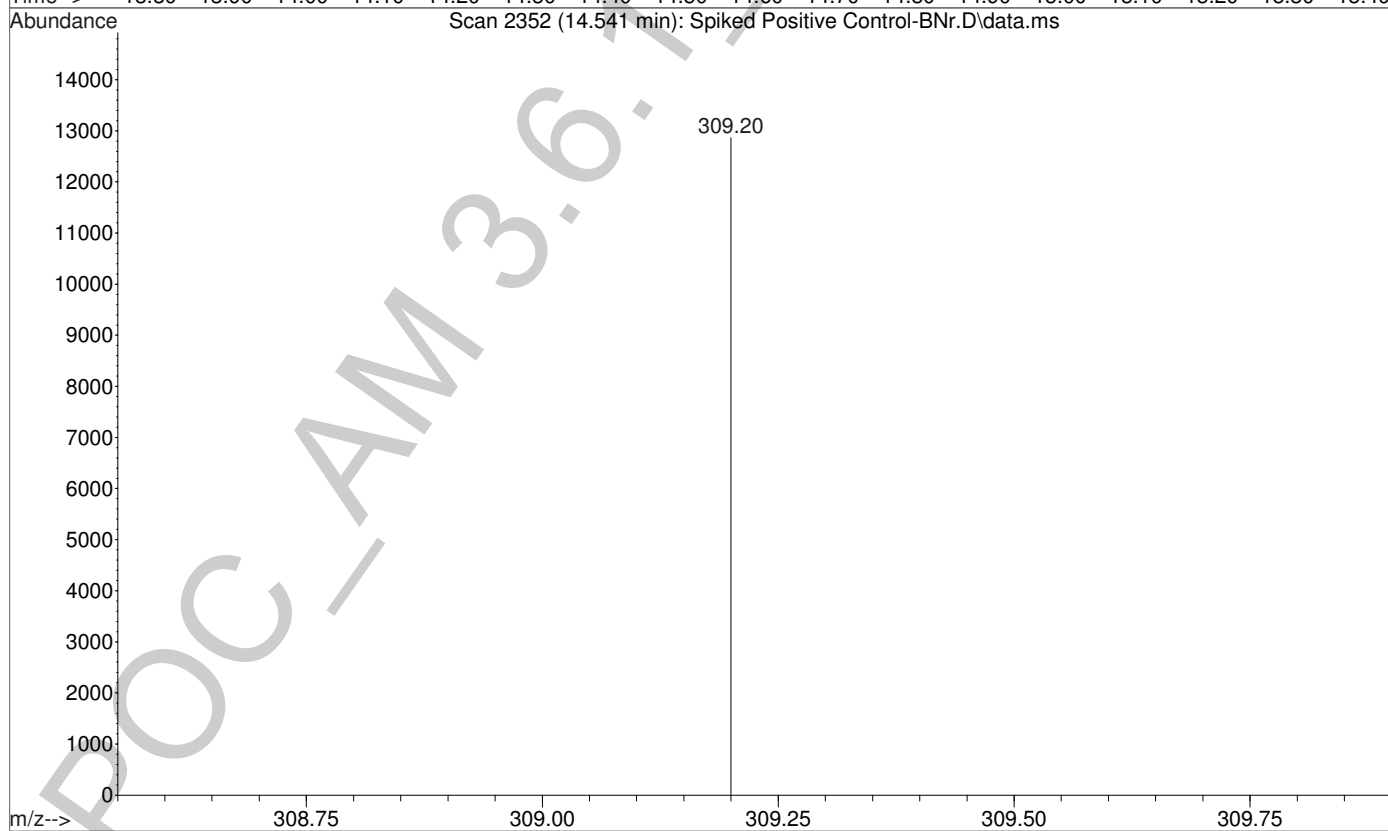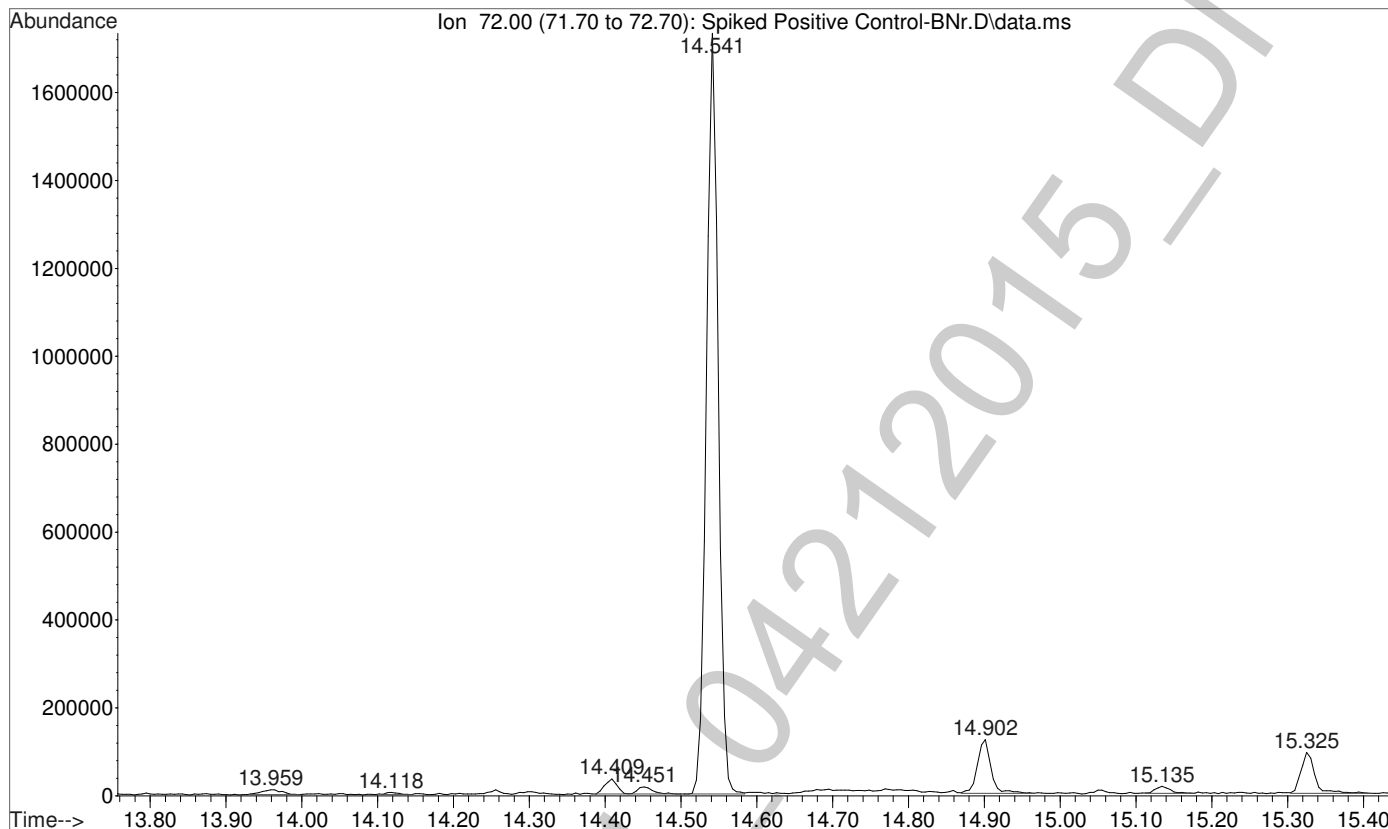



File :C:\gcms\1\data\Blood\042115BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 21 Apr 2015 14:01 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

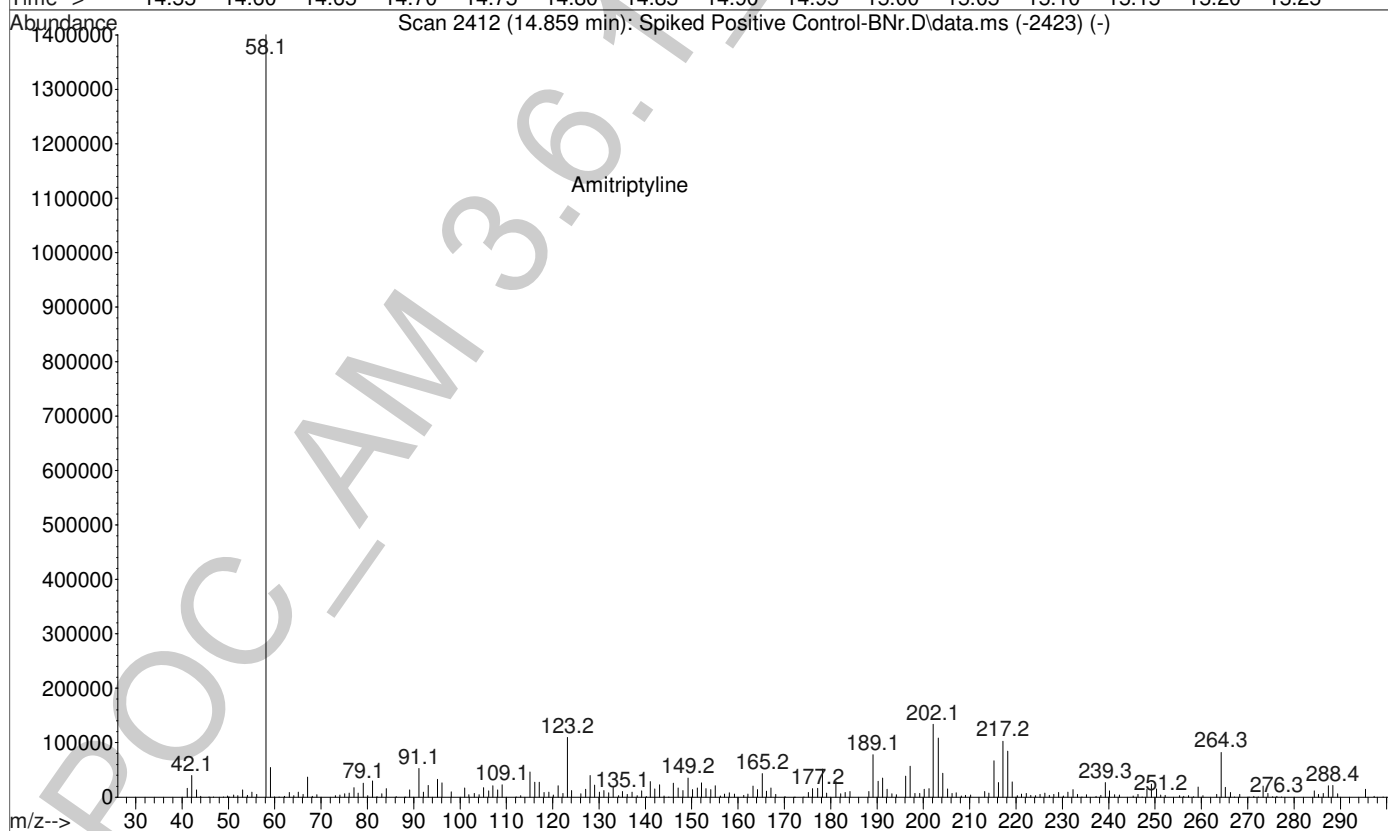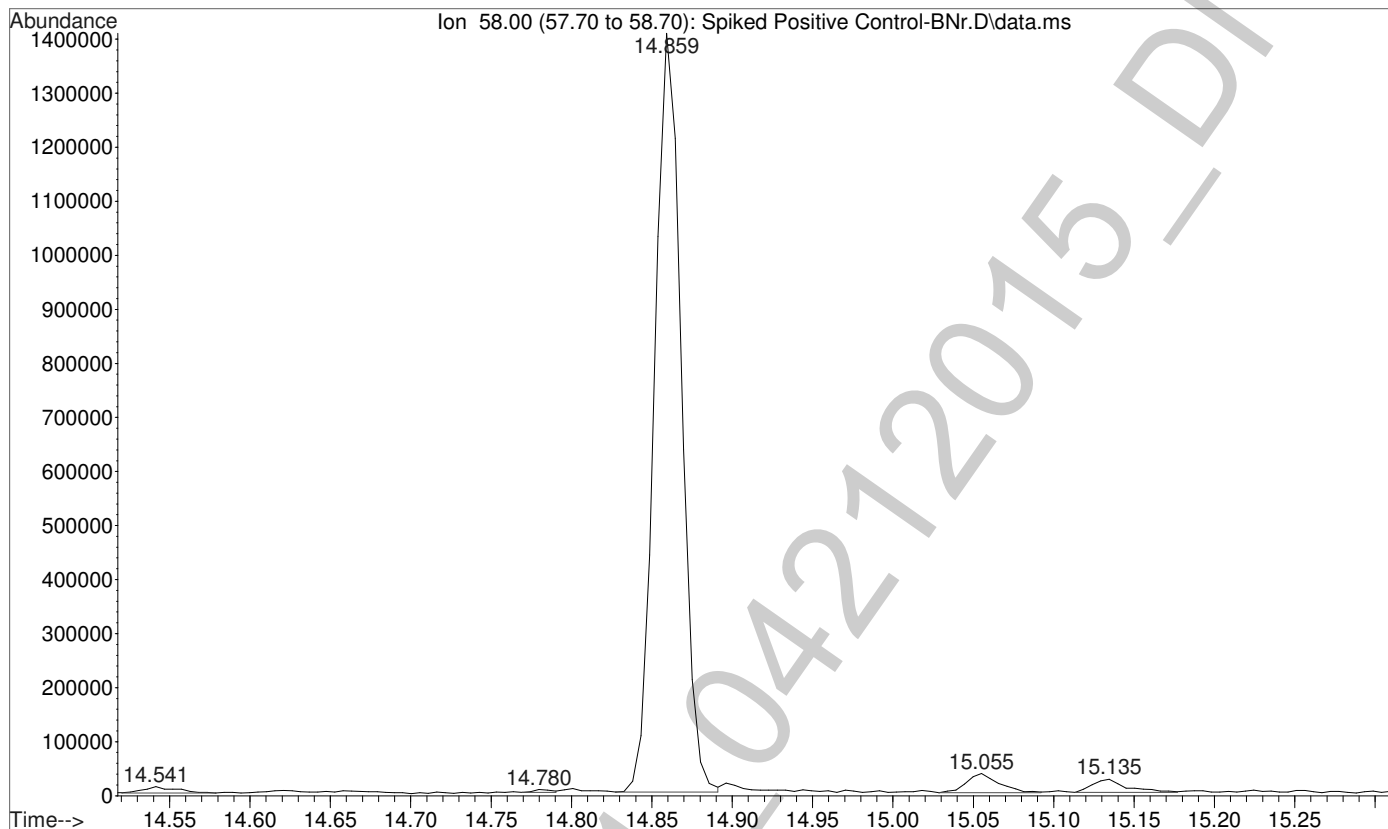



File :C:\gcms\1\data\Blood\042115BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 21 Apr 2015 14:01 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

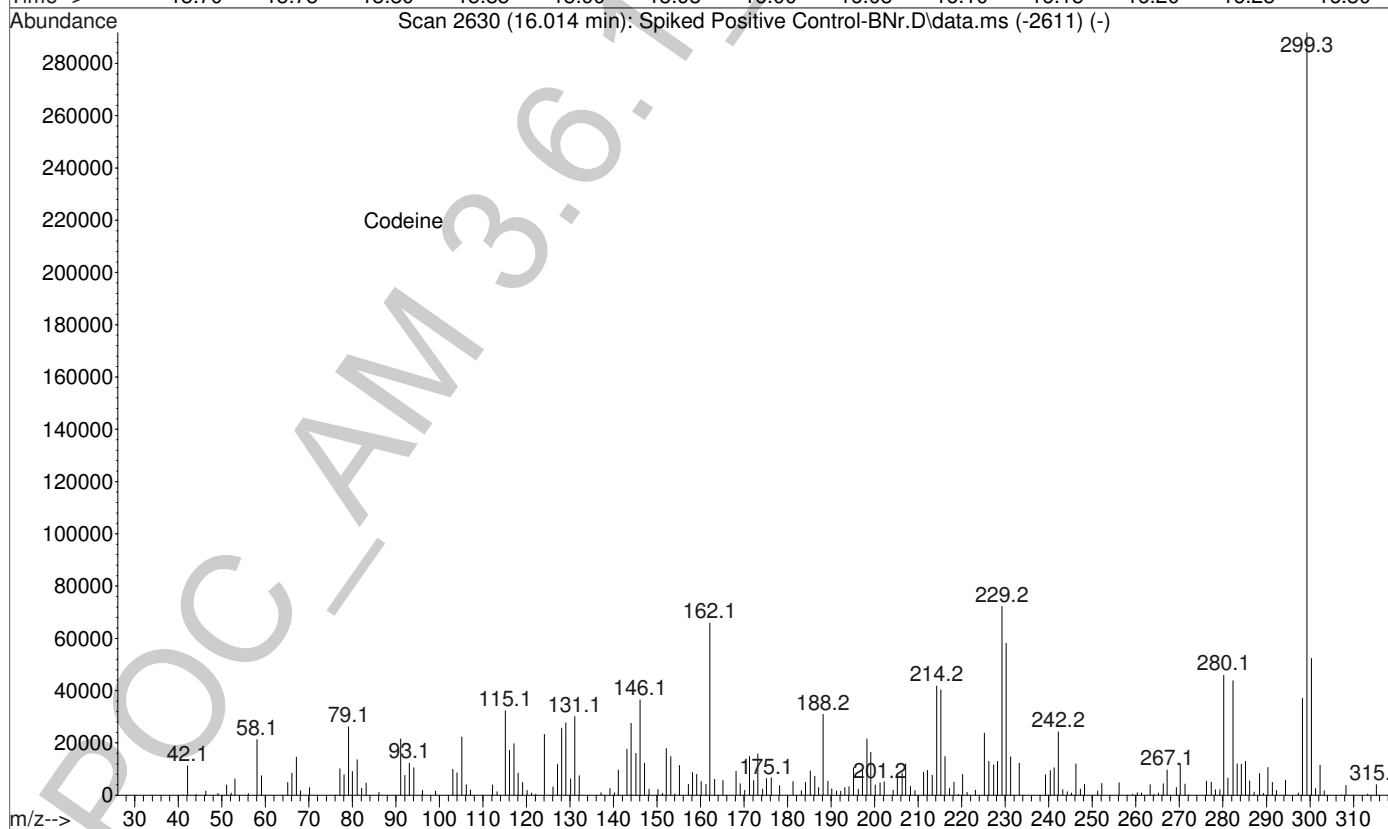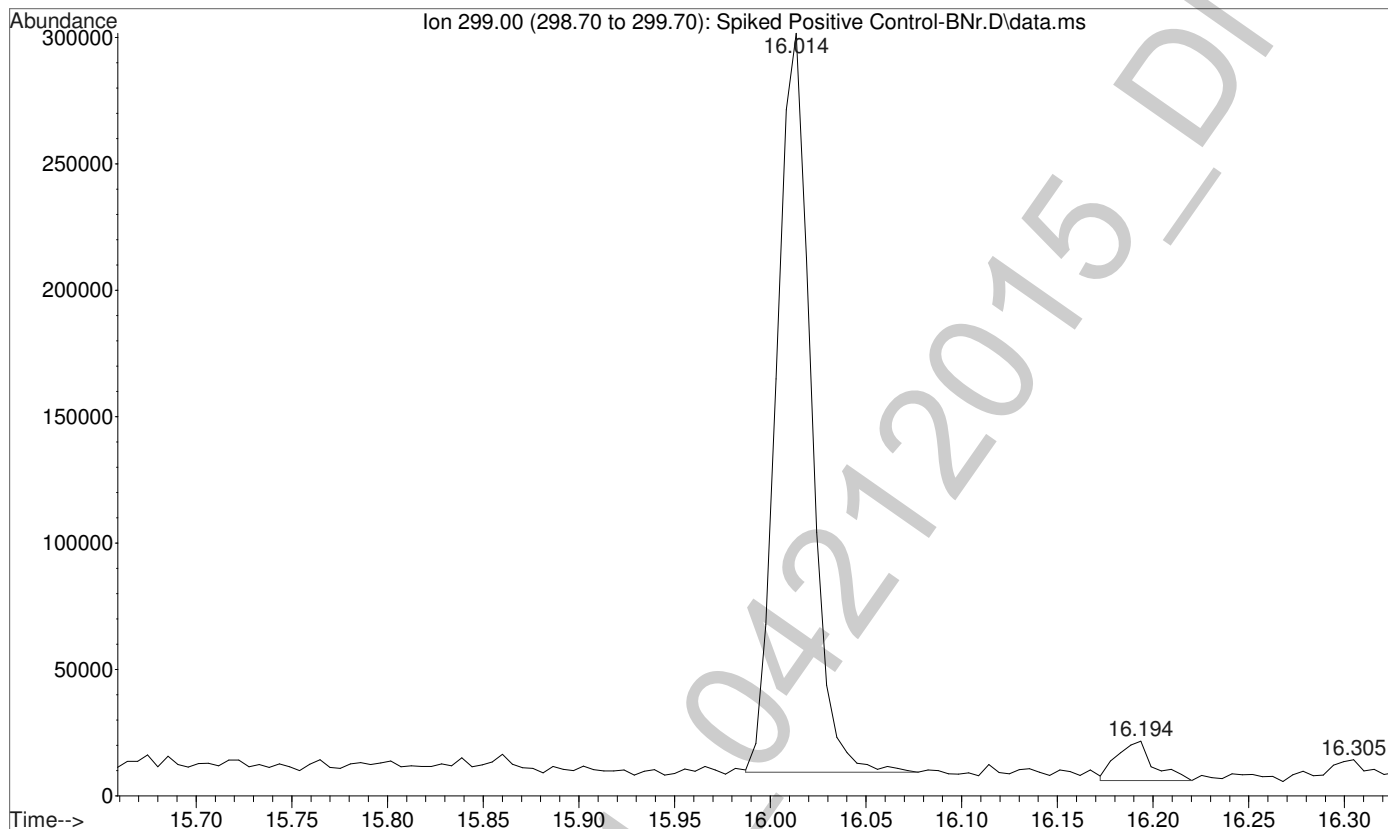



File :C:\gcms\1\data\Blood\042115BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 21 Apr 2015 14:01 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

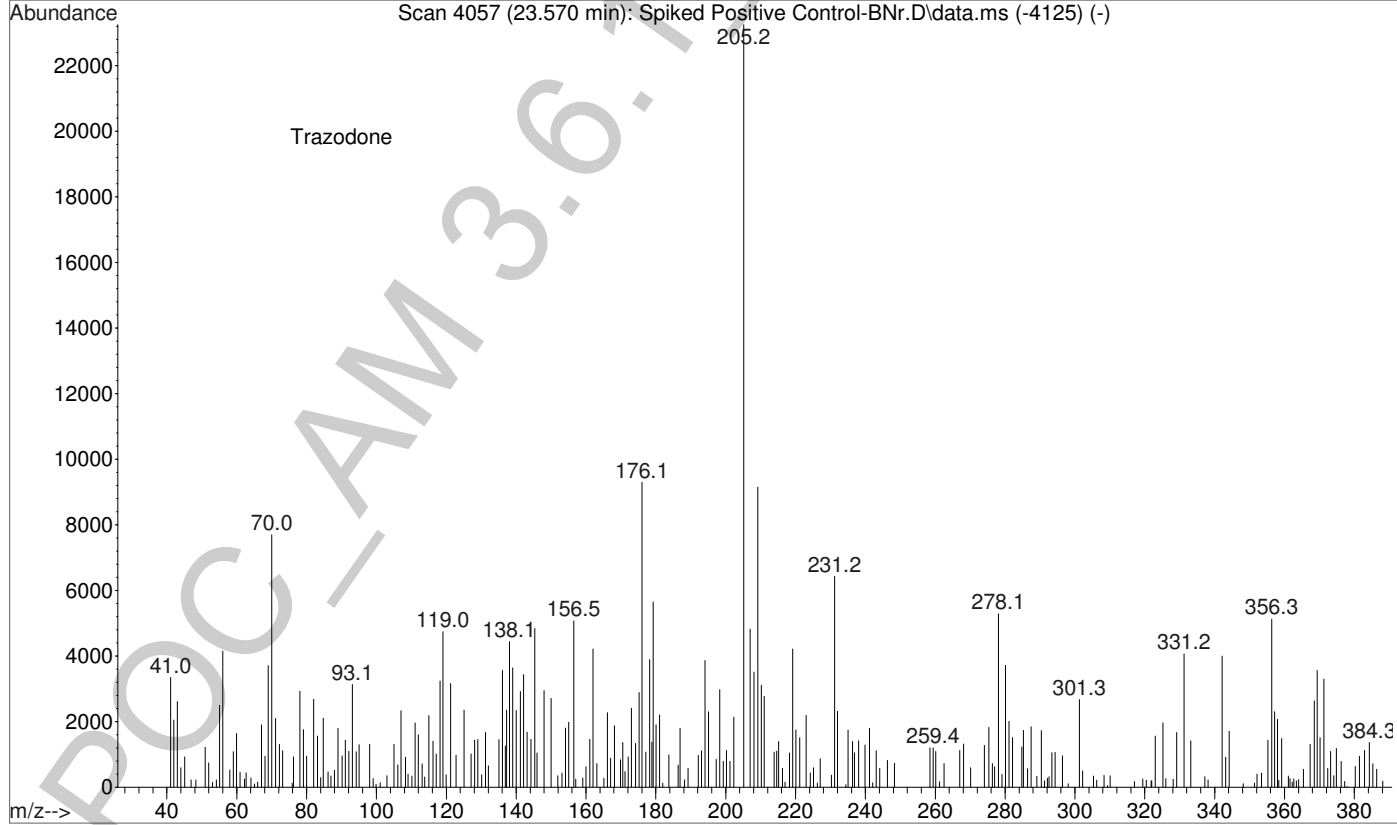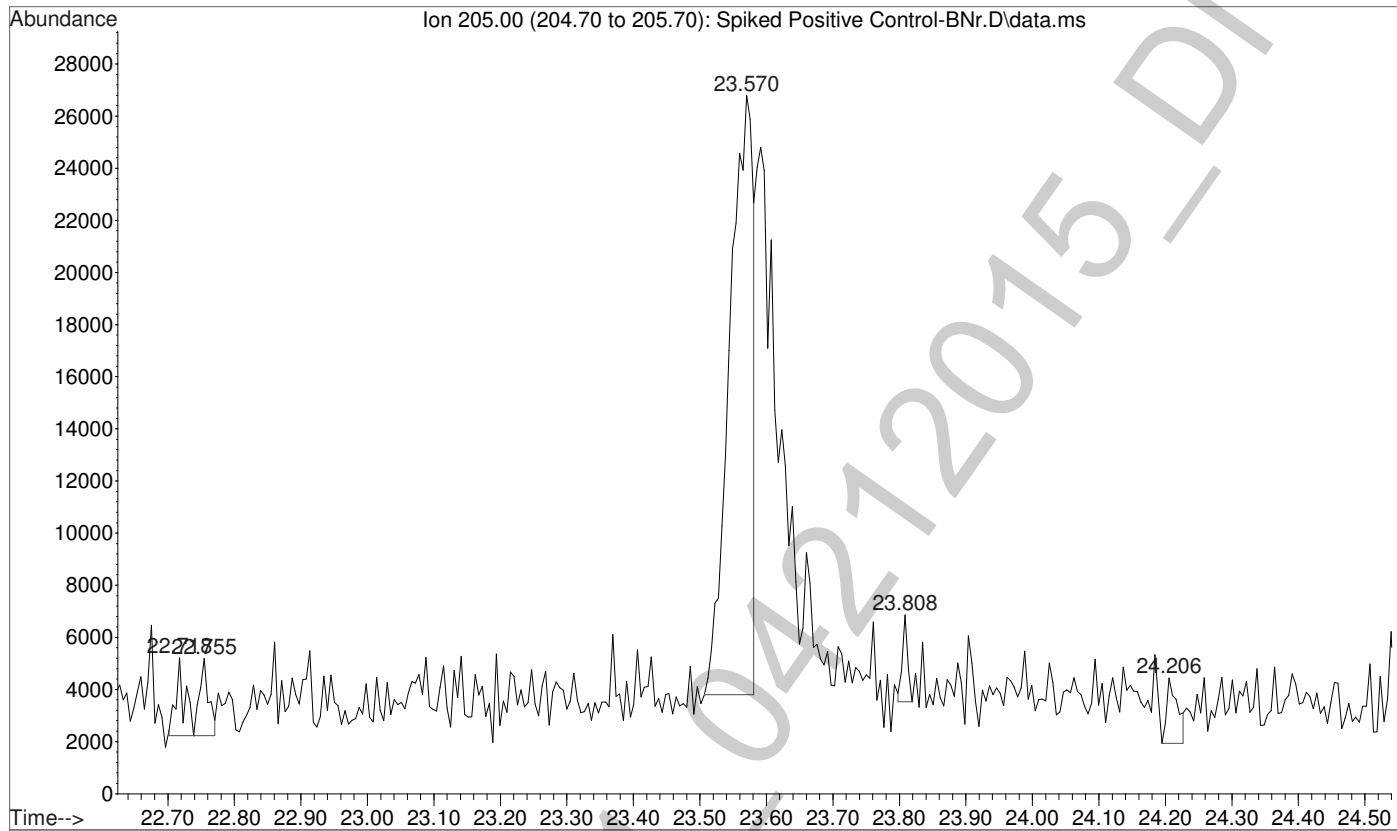

File :C:\gcms\1\data\Blood\042115BN\Reinjection Longer GC Method\p
... rbLK2r.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 21 Apr 2015 14:35 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Solvent Blank
Misc Info : Chloroform

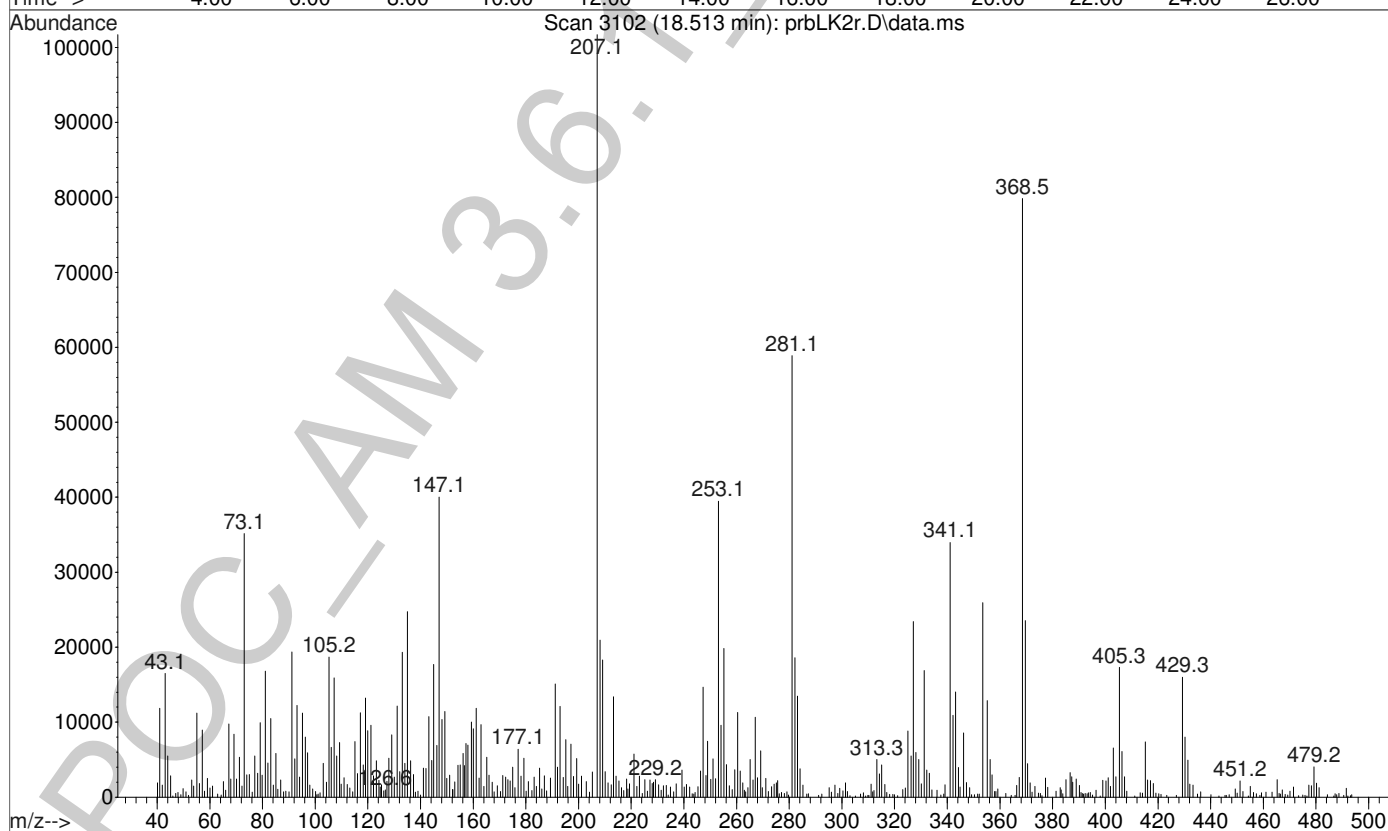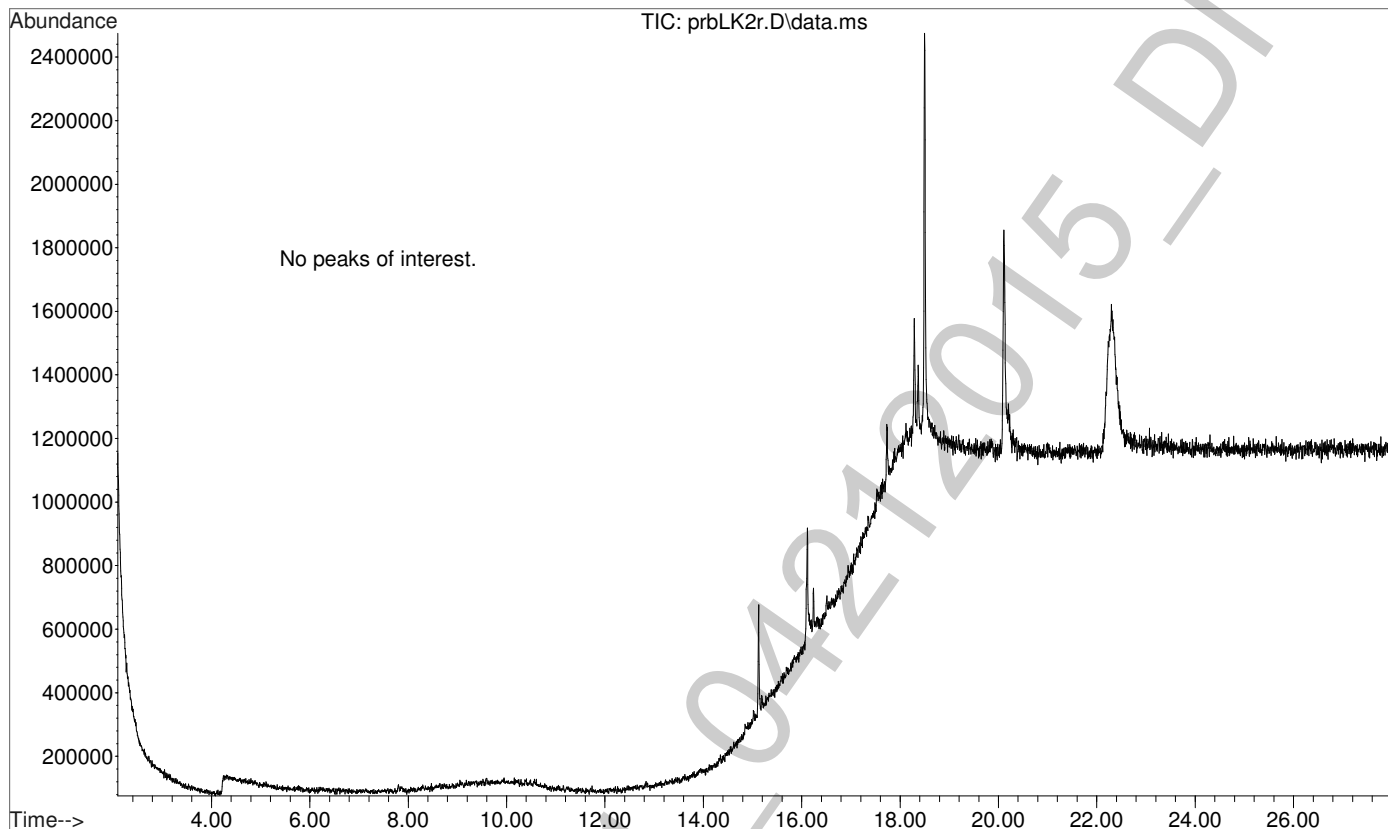

File :C:\gcms\1\data\Blood\042115BN\Reinjection Longer GC Method\P
... OSTBLKr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 24 Apr 2015 16:11 using AcqMethod BNSB120510.M
Sample Name: BLK
Misc Info : Chloroform

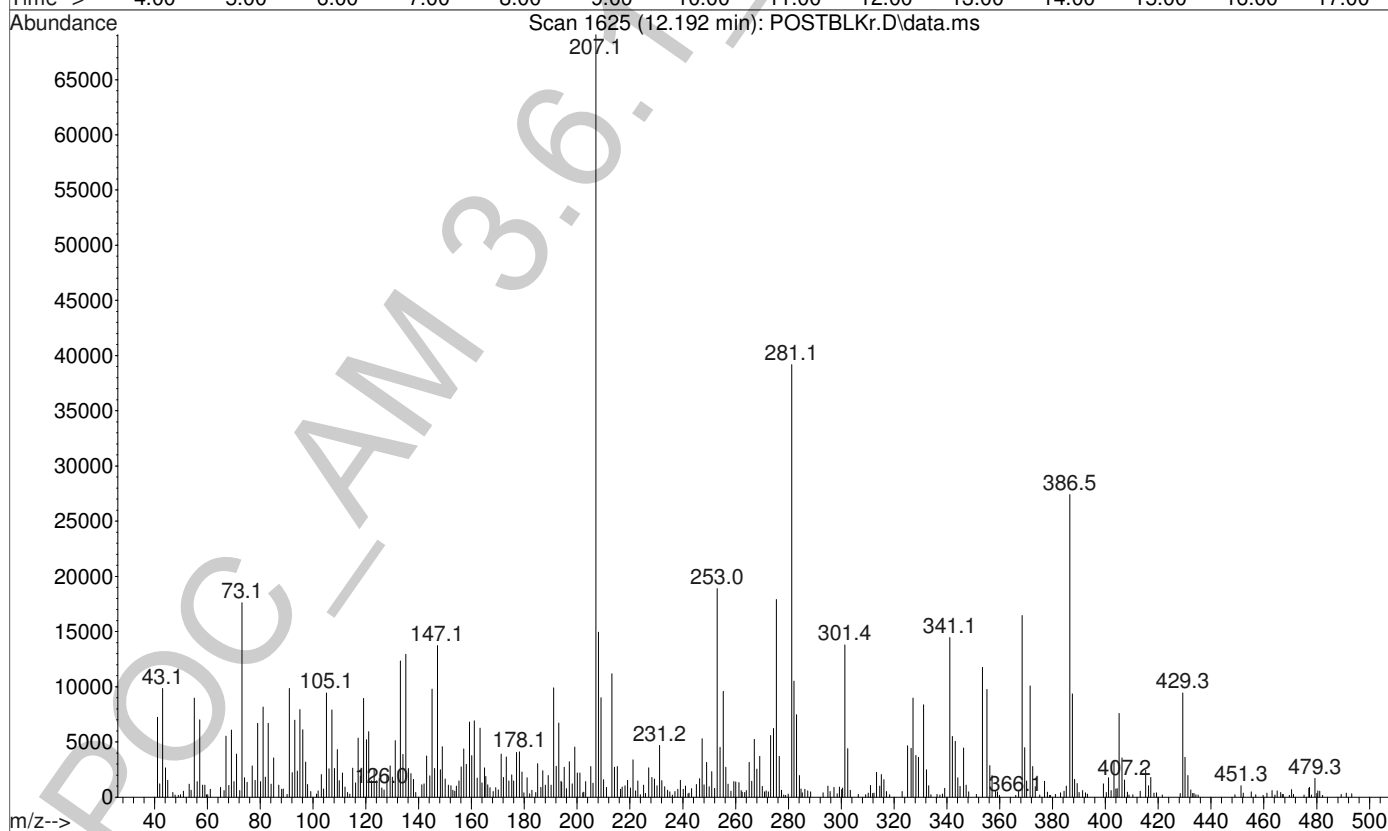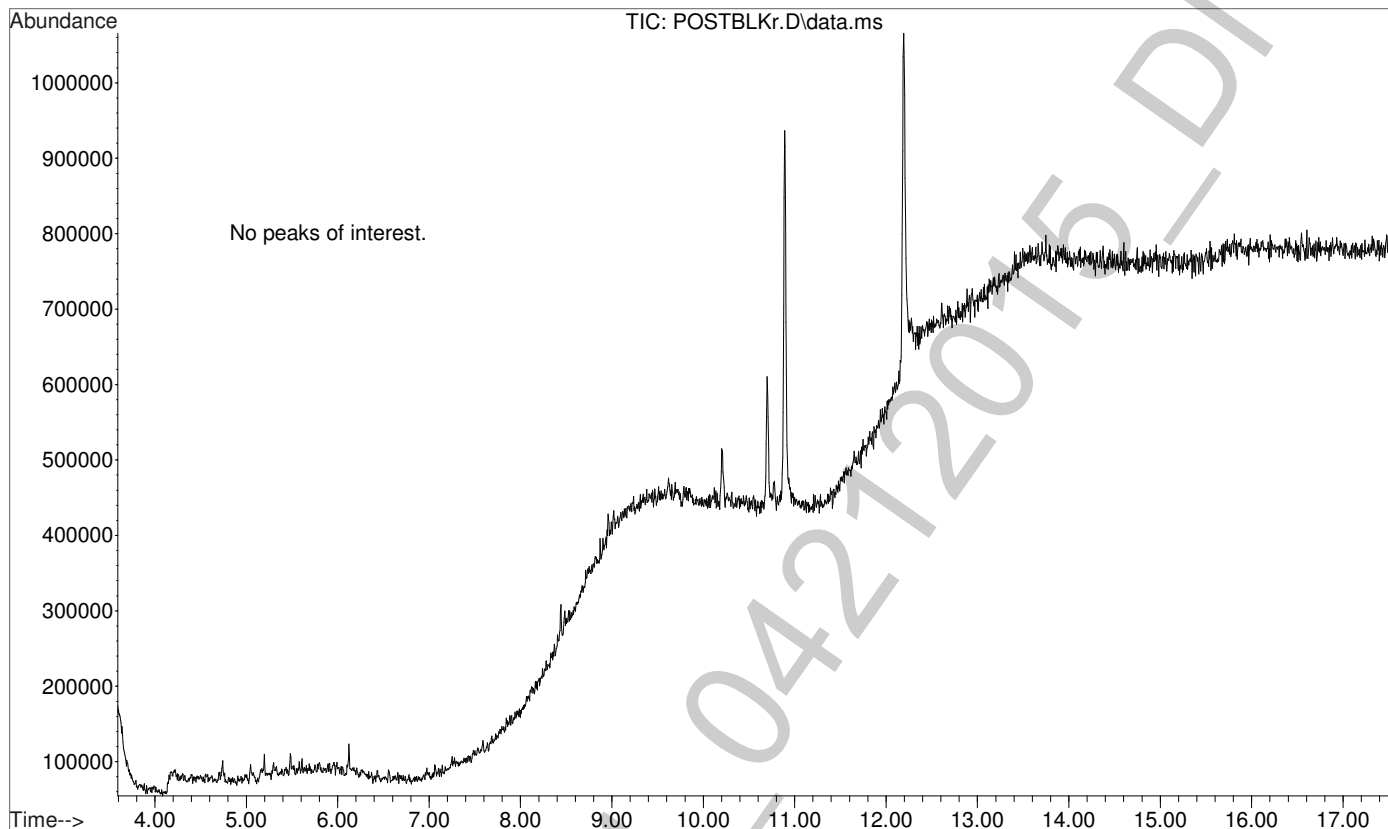

File :C:\gcms\1\data\Blood\042115BN\AFTER.D
Operator : 5LAB-C01\ISPuser
Acquired : 24 Apr 2015 16:34 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: BLK
Misc Info : Chloroform
Vial Number: 64

