

Worklist: 699

<u>LAB CASE</u>	<u>ITEM</u>	<u>TASK ID</u>	<u>DESCRIPTION</u>	
M2015-1133	2	31796	3.6.1 Blood base neutral confirr	
M2015-1152	2	32635	3.6.1 Blood base neutral confirr	
M2015-1161	1	31757	3.6.1 Blood base neutral confirr	
M2015-1172	1	31831	3.6.1 Blood base neutral confirr	
M2015-1227	1	32095	3.6.1 Blood base neutral confirr	
M2015-1237	1	32152	3.6.1 Blood base neutral confirr	
M2015-1257	1	32613	3.6.1 Blood base neutral confirr	
M2015-1259	1	32269	3.6.1 Blood base neutral confirr	
M2015-1260	1	32274	3.6.1 Blood base neutral confirr	
M2015-1261	1	32279	3.6.1 Blood base neutral confirr	
M2015-1273	1	32331	3.6.1 Blood base neutral confirr	
M2015-1318	2	32725	3.6.1 Blood base neutral confirr	
M2015-1353	3	32718	3.6.1 Blood base neutral confirr	
P2015-1011	1	32418	3.6.1 Blood base neutral confirr	
P2015-1025	1	32588	3.6.1 Blood base neutral confirr	
P2015-1028	1	32648	3.6.1 Blood base neutral confirr	
P2015-1042	1	32722	3.6.1 Blood base neutral confirr	
P2015-1043	1	32736	3.6.1 Blood base neutral confirr	
P2015-1060	1	32884	3.6.1 Blood base neutral confirr	
P2015-1063	1	32892	3.6.1 Blood base neutral confirr	
P2015-1064	1	32934	3.6.1 Blood base neutral confirr	
P2015-1065	1	32940	3.6.1 Blood base neutral confirr	
P2015-1066	1	32945	3.6.1 Blood base neutral confirr	

POC-AM361050527

g

Worklist: 699

<u>LAB_CASE</u>	<u>ITEM</u>	<u>TASK_ID</u>	<u>DESCRIPTION</u>
P2015-1067	1	32954	3.6.1 Blood base neutral confirr
P2015-1068	1	33001	3.6.1 Blood base neutral confirr



POC_AM 3.6.1_05052015_CSS

Analytical Method 3.6.1 & 3.6.7 QA Check List

Run Start Date: 05/05/15

Analyst: CS

(Short GC/MS temperature program)

Positive Control Compound List

- Methamphetamine
- Nicotine
- Meperidine
- Caffeine
- Diphenhydramine
- Lidocaine
- PCP
- Methadone
- Amitriptyline
- Codeine
- Trazodone



Internal Standards

- Benzphetamine
- Papaverine

Optional back extraction **not** performed.
Reconstituted in MeOH.



File :F:\Data\050515\Prerun Solvent Blank.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 17:53 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Pre-run Solvent Blank
Misc Info : Chloroform
Vial Number: 100

2

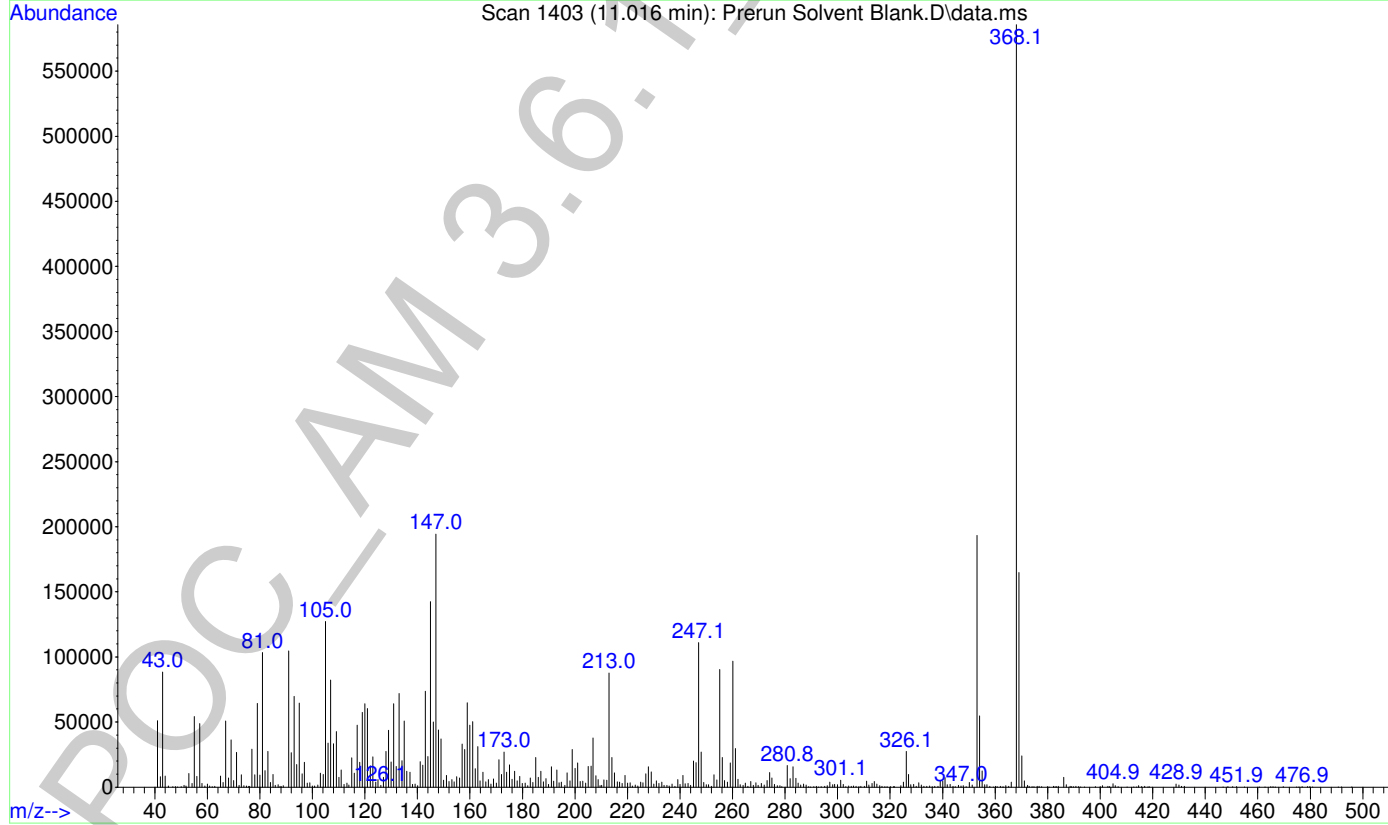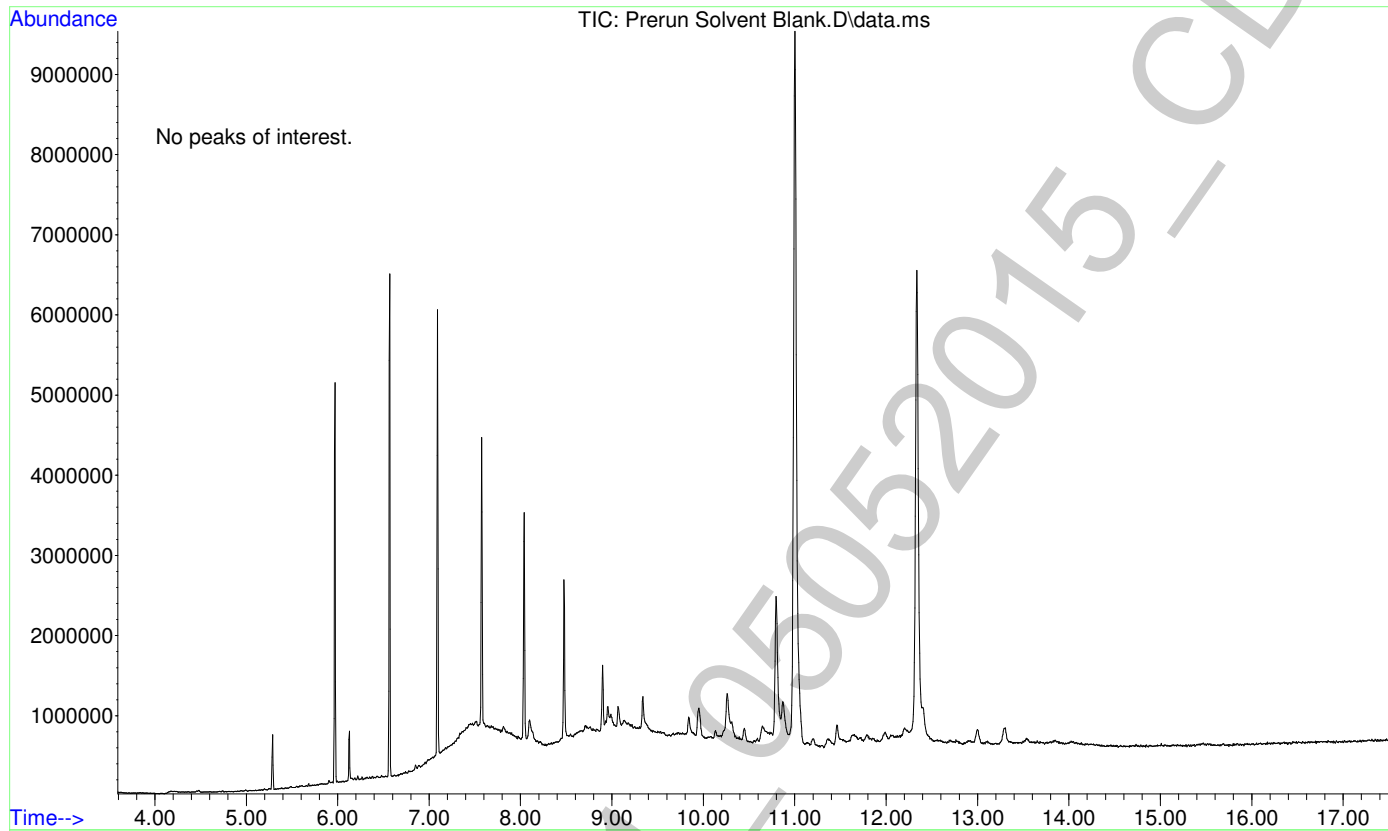


2

File :F:\Data\050515\prbLK2.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 19:03 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Solvent Blank
Misc Info : Chloroform
Vial Number: 99

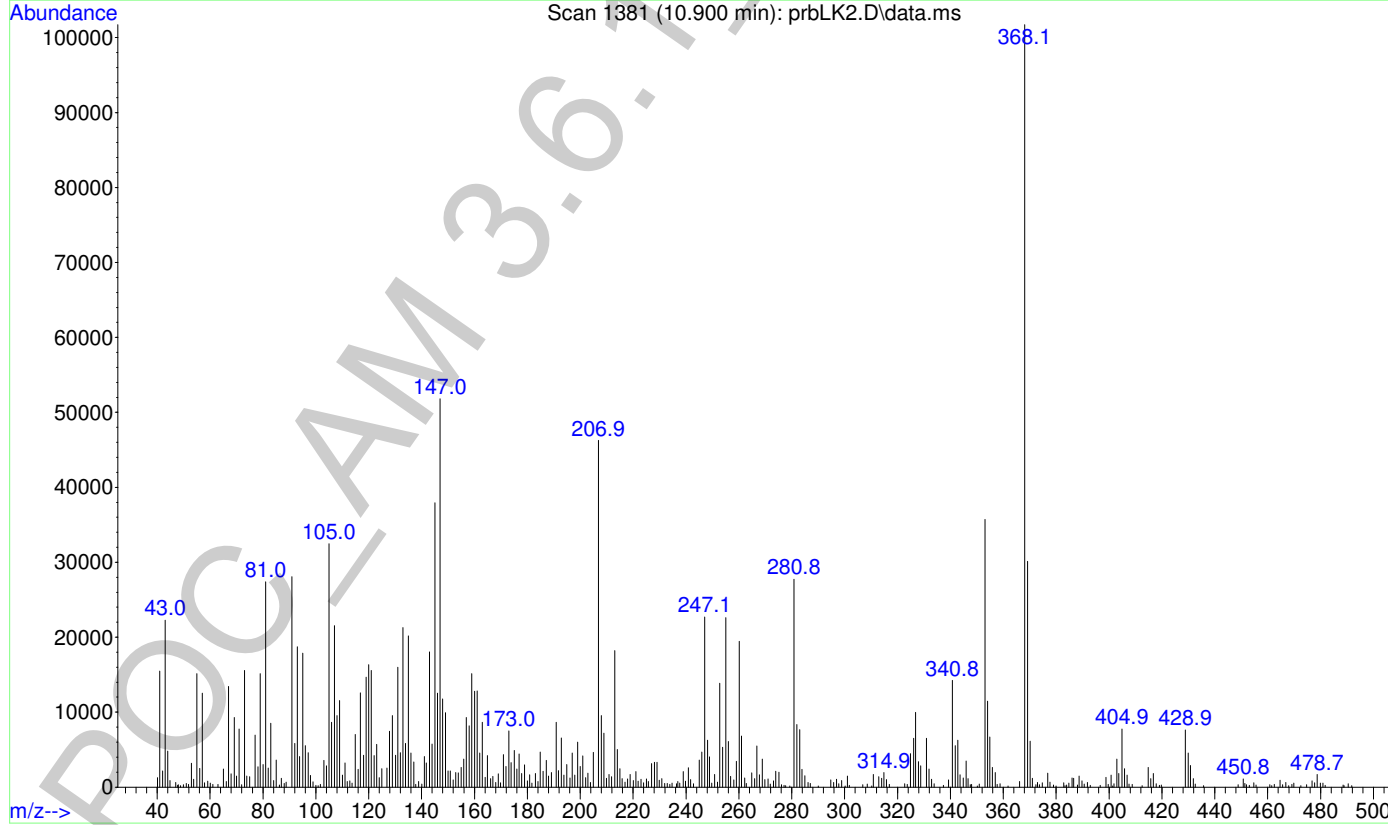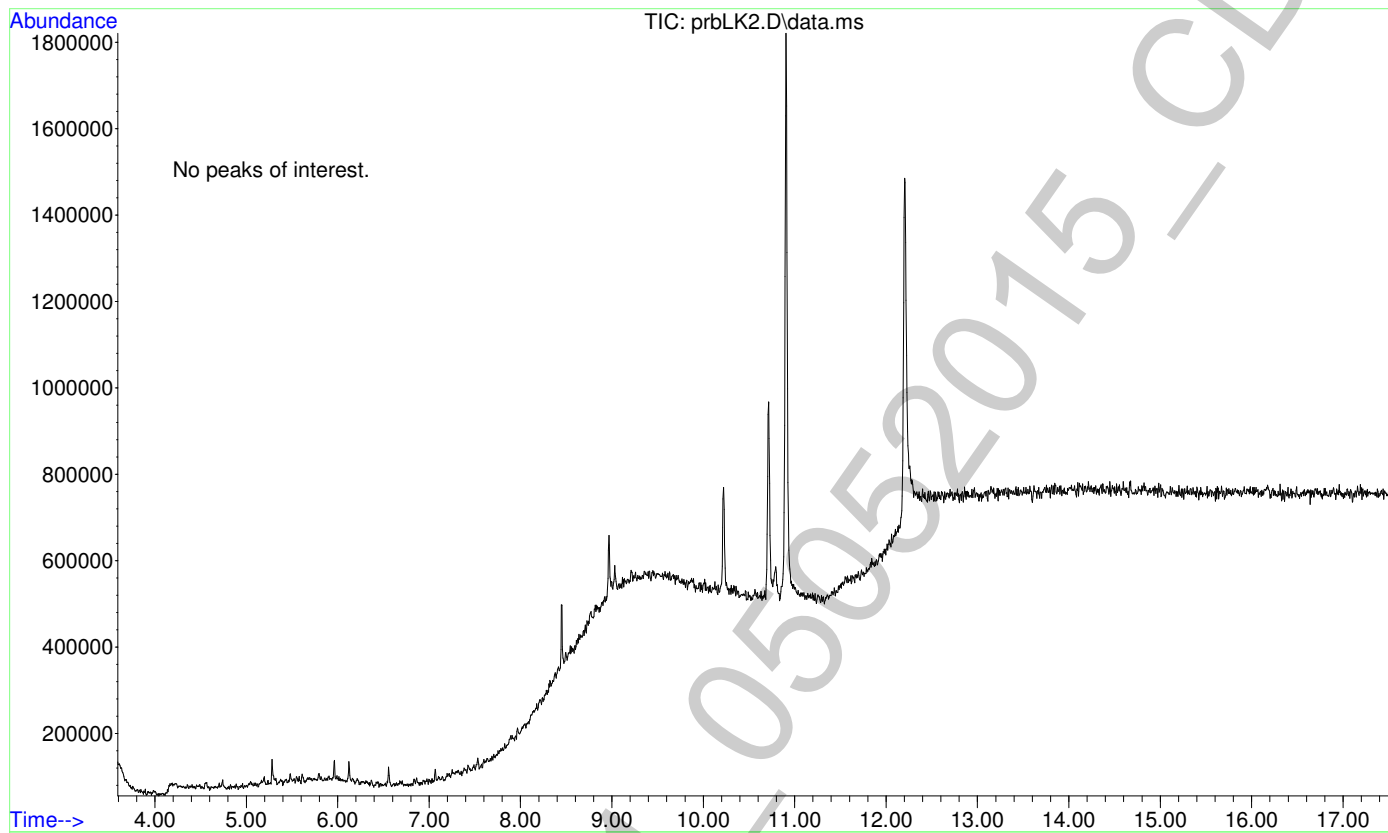



2

File :F:\Data\050515\Negative Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 18:16 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1
Vial Number: 1

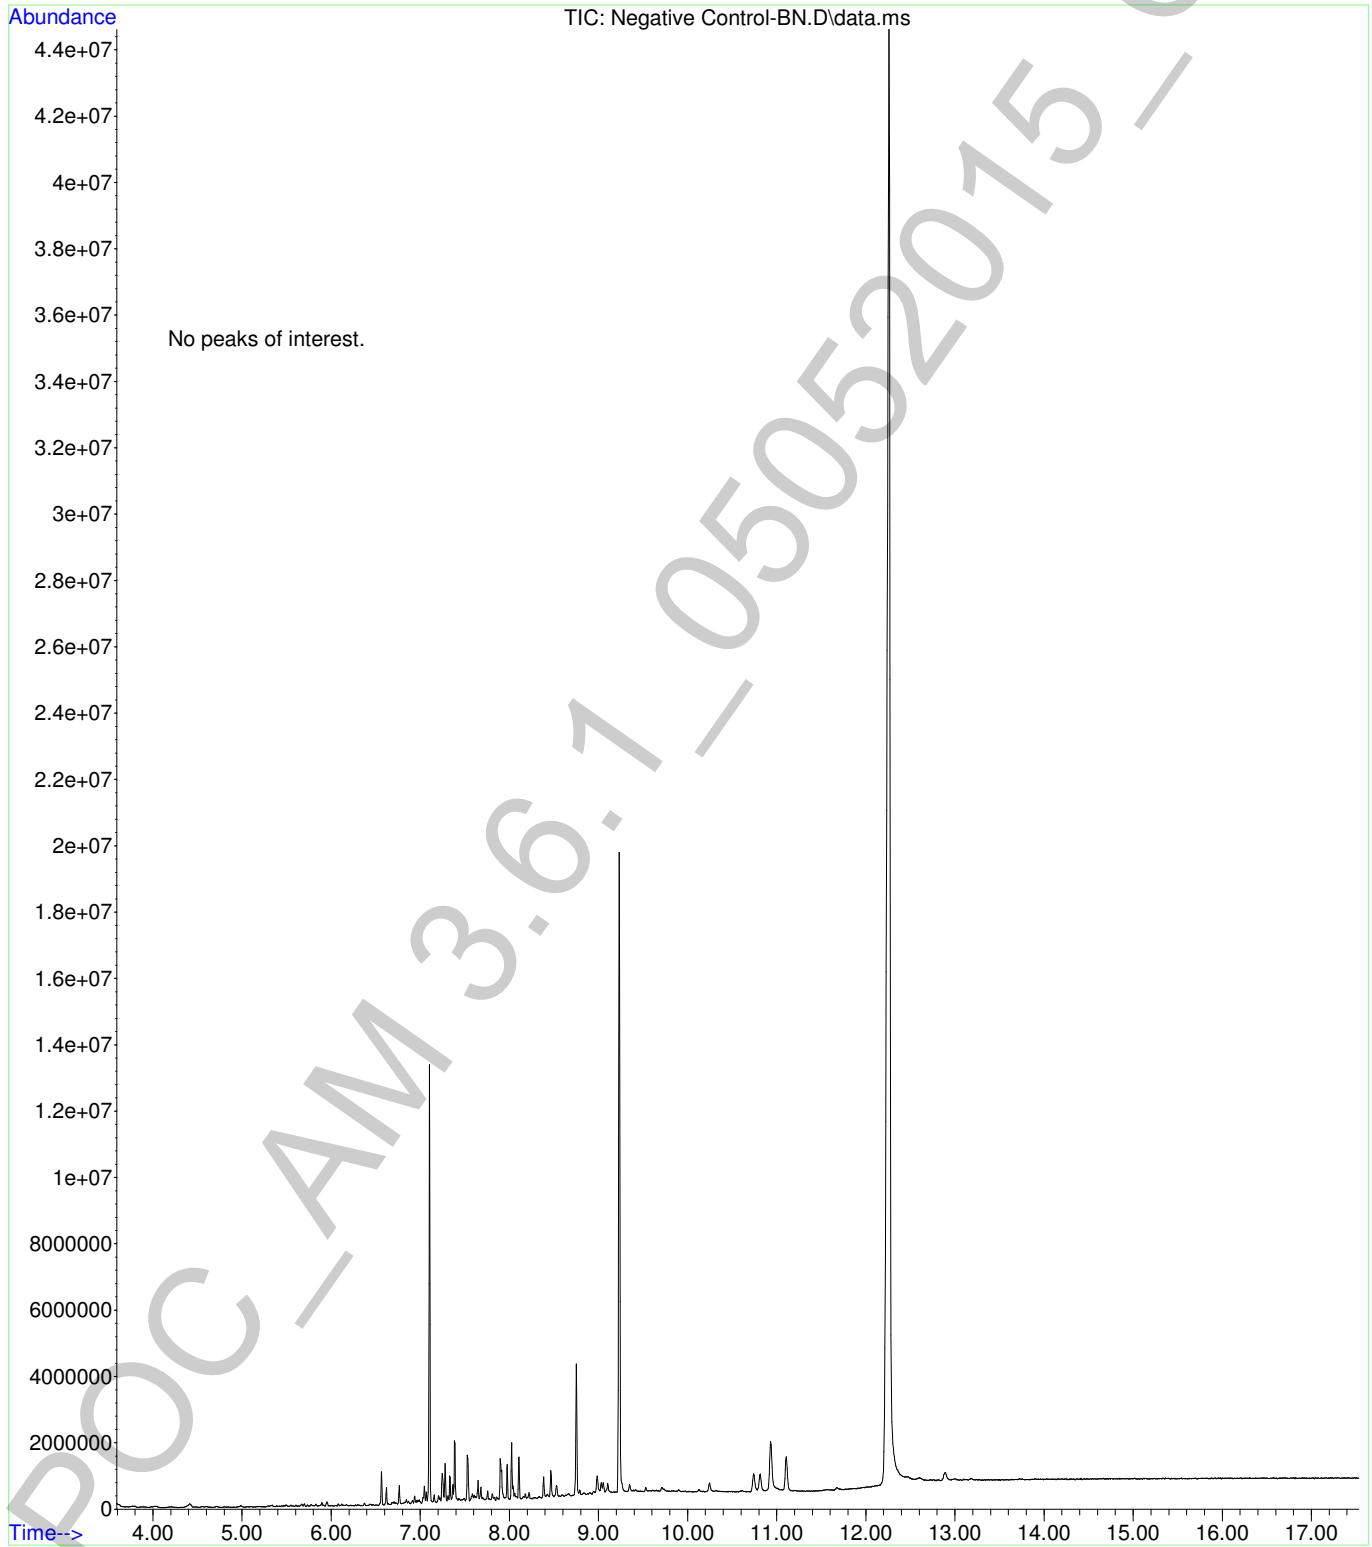



File :F:\Data\050515\Negative Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 18:16 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1
Vial Number: 1

6

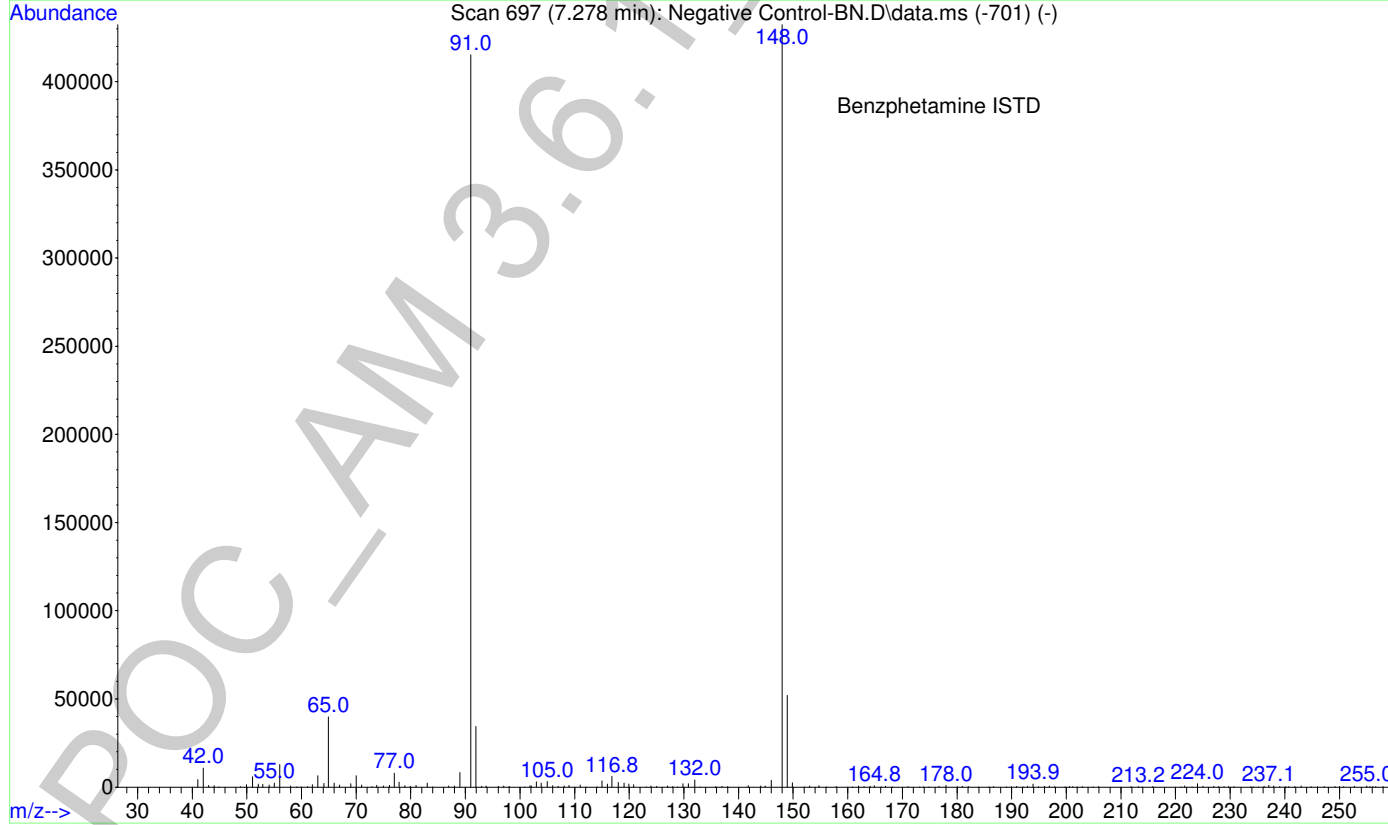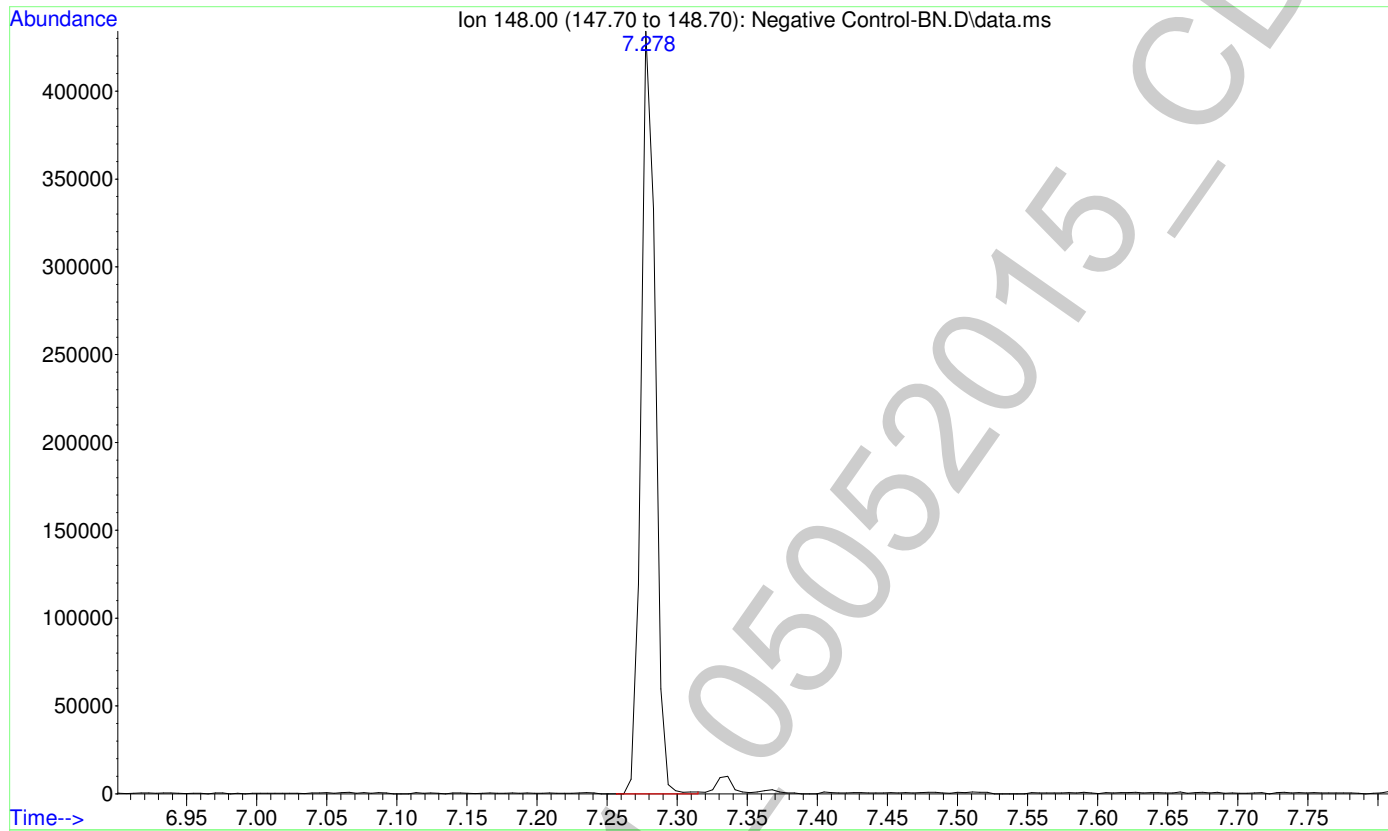


File :F:\Data\050515\Negative Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 18:16 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1
Vial Number: 1

2

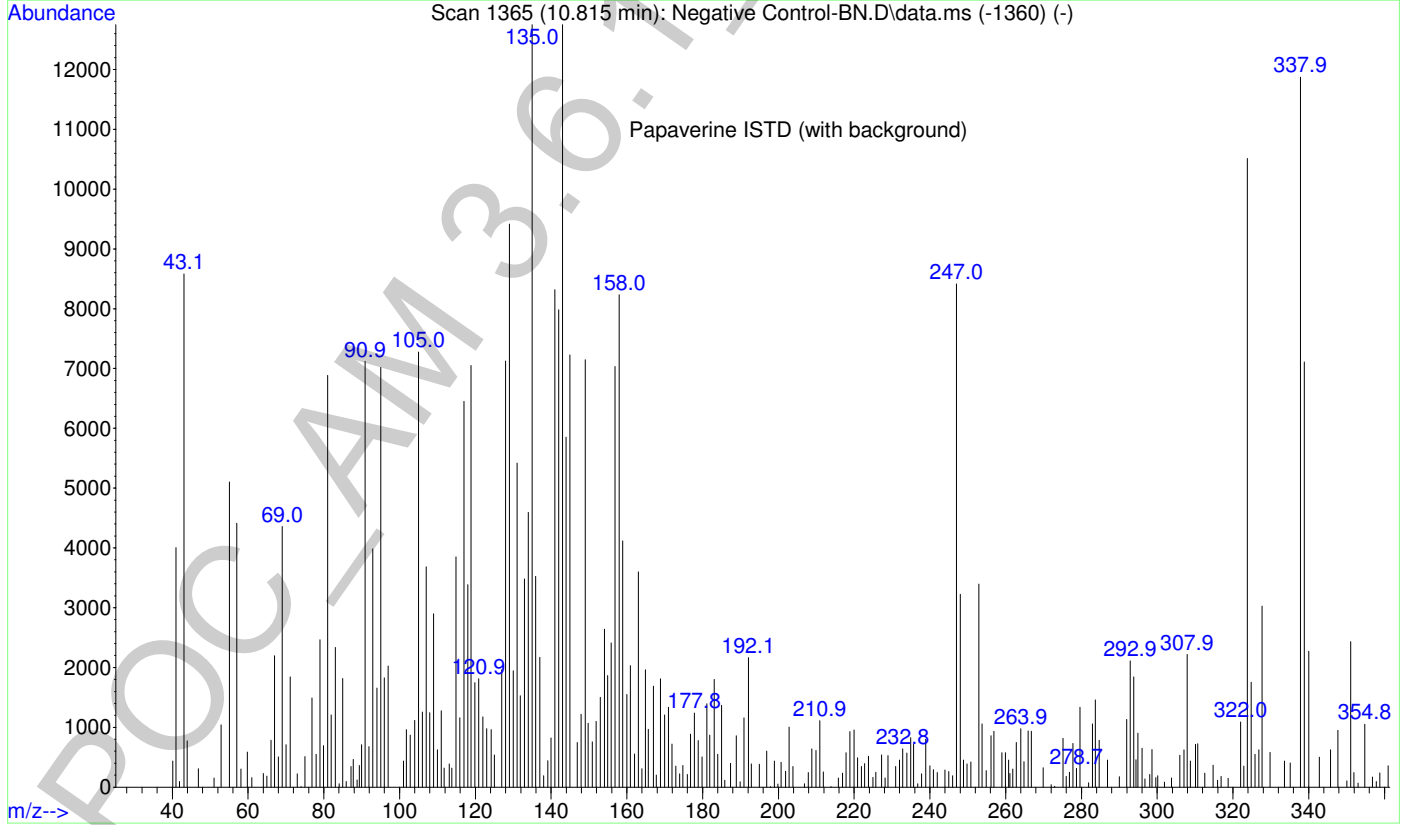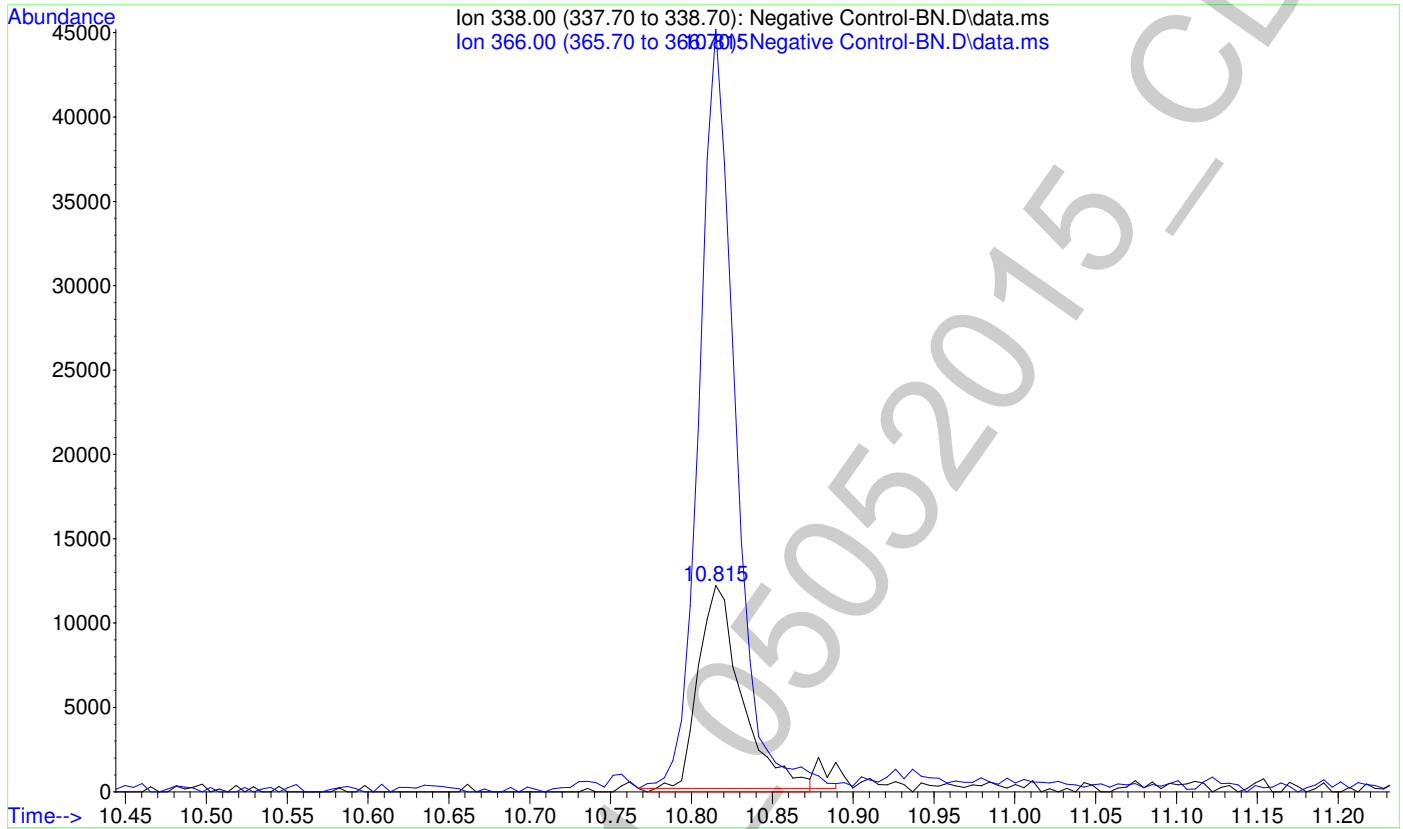



2

File :F:\Data\050515\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 18:39 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

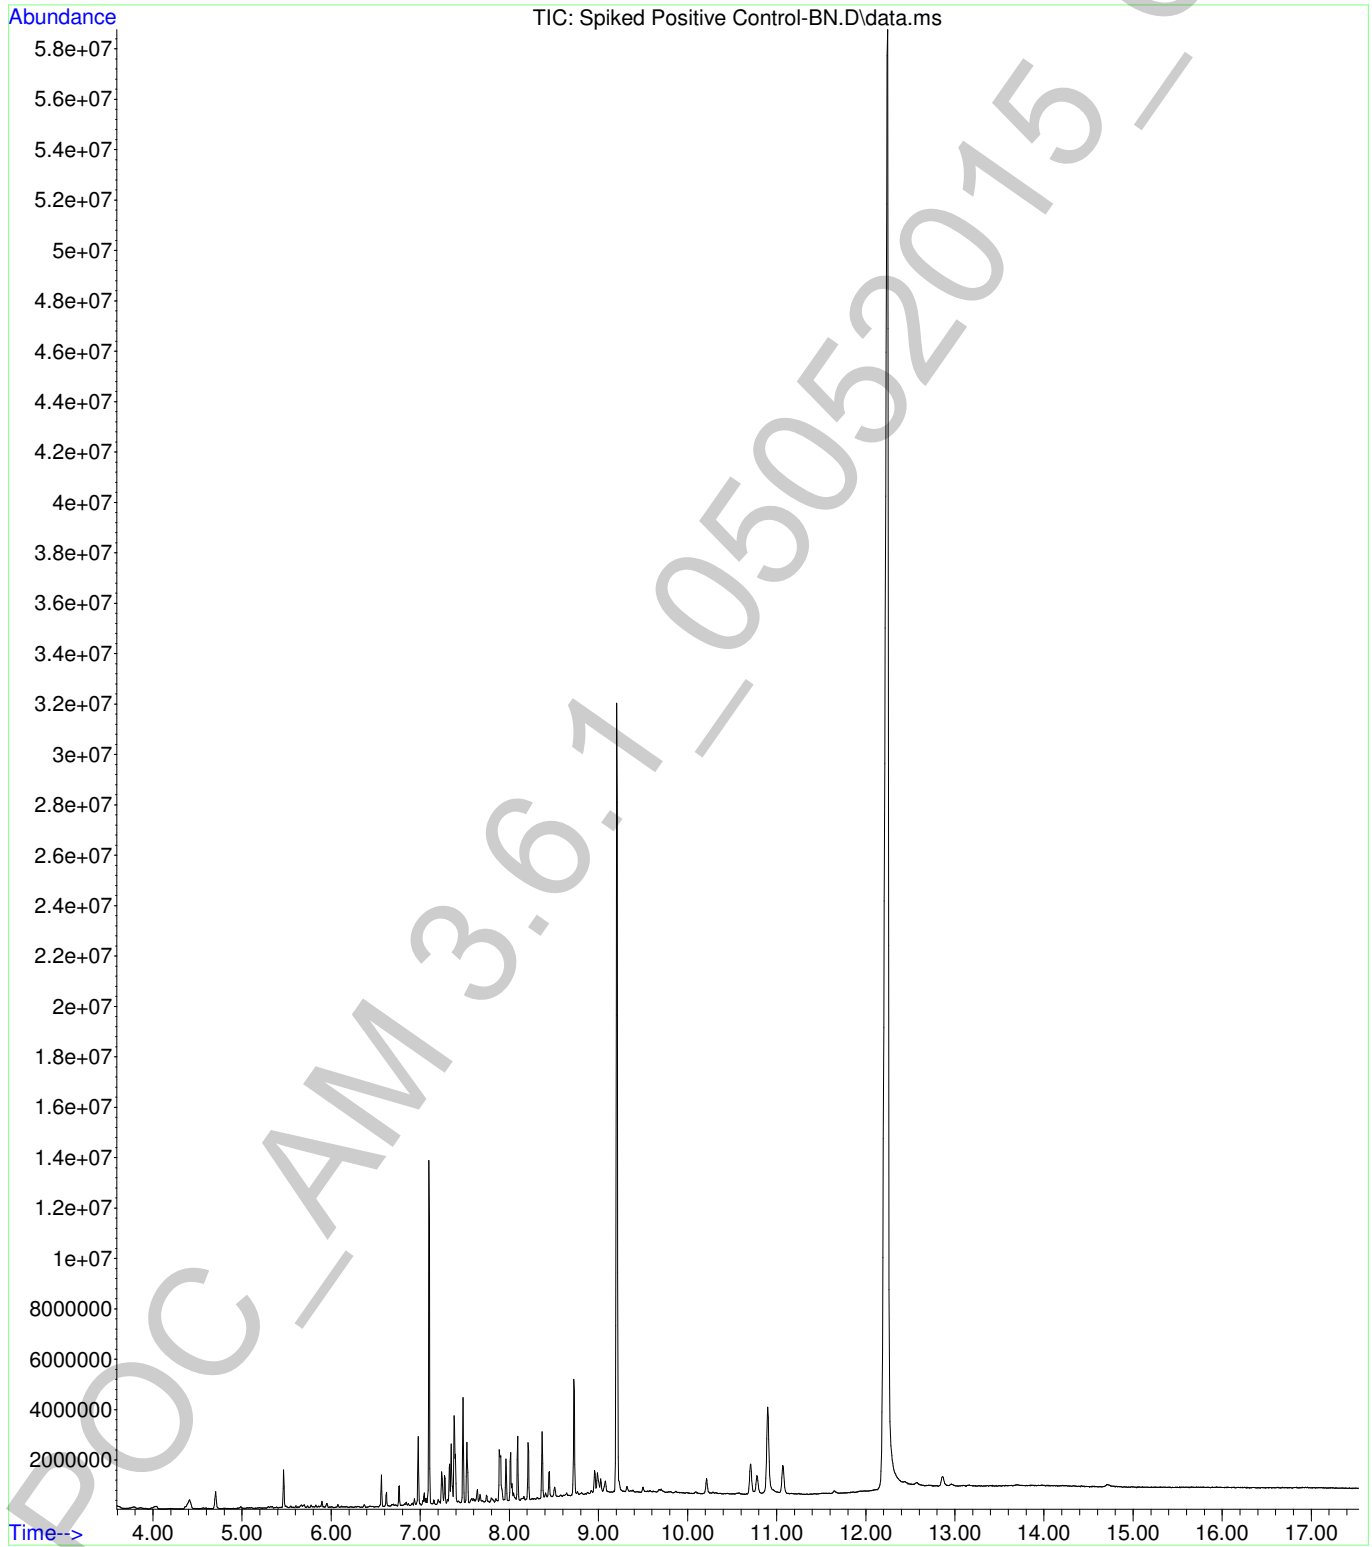



6

File :F:\Data\050515\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 18:39 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

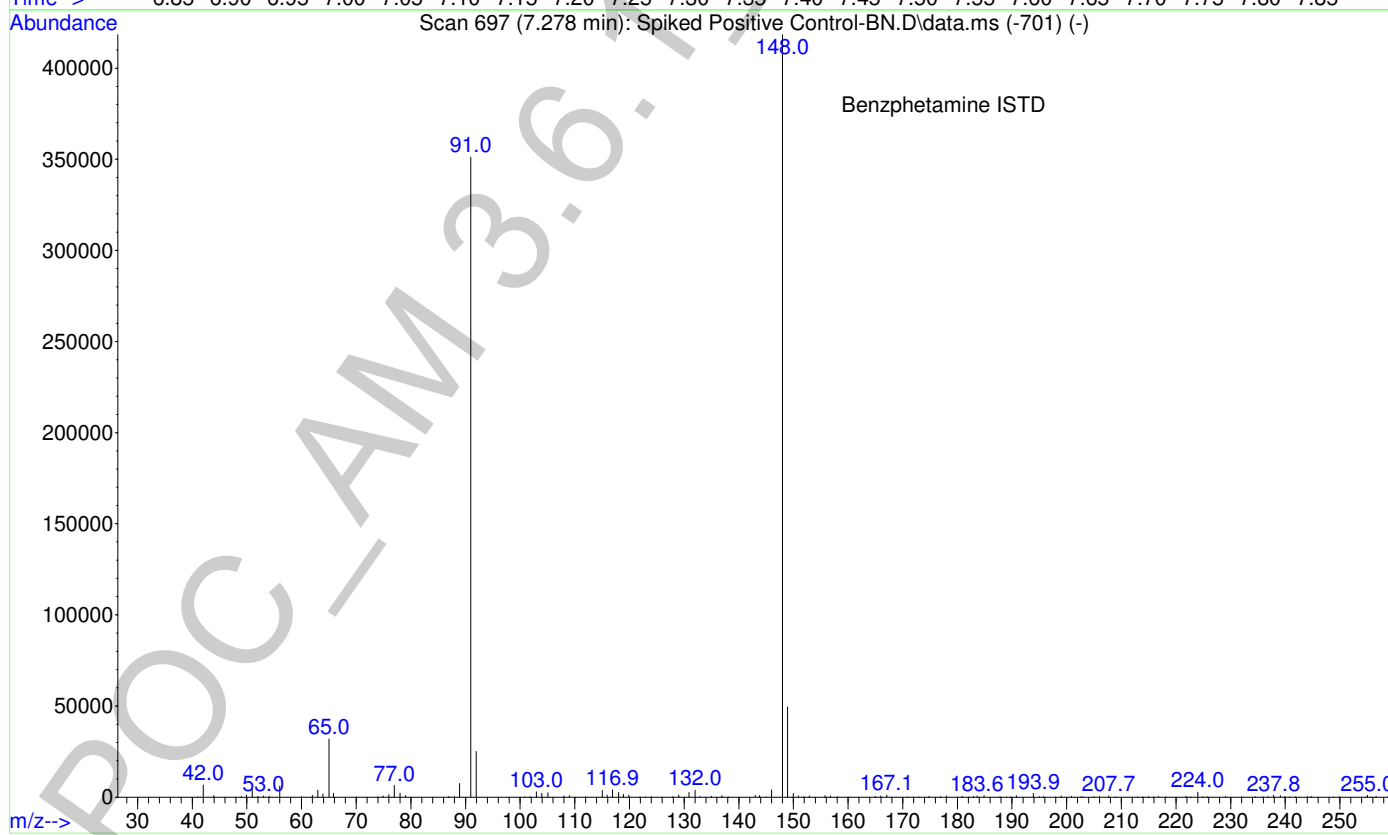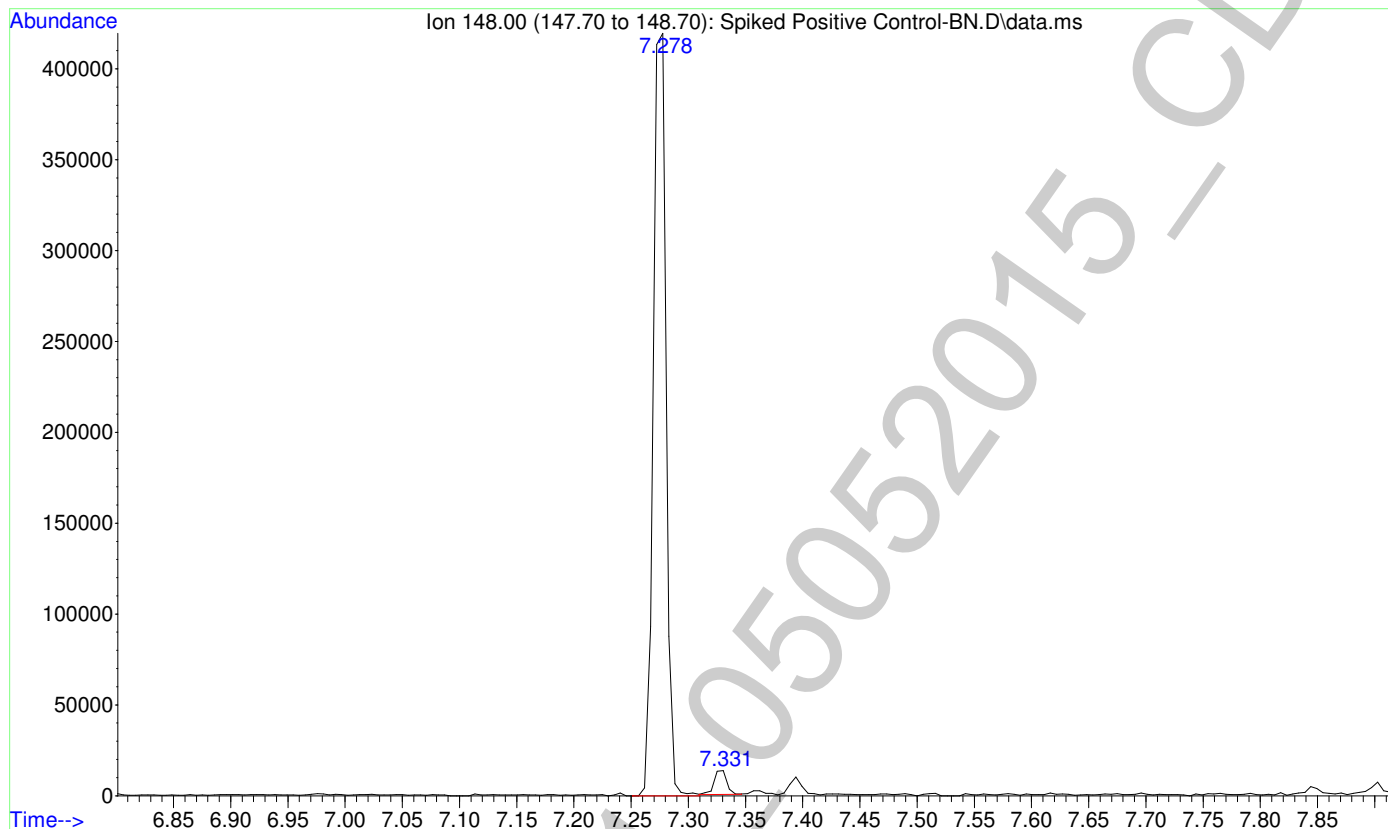



2

File :F:\Data\050515\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 18:39 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

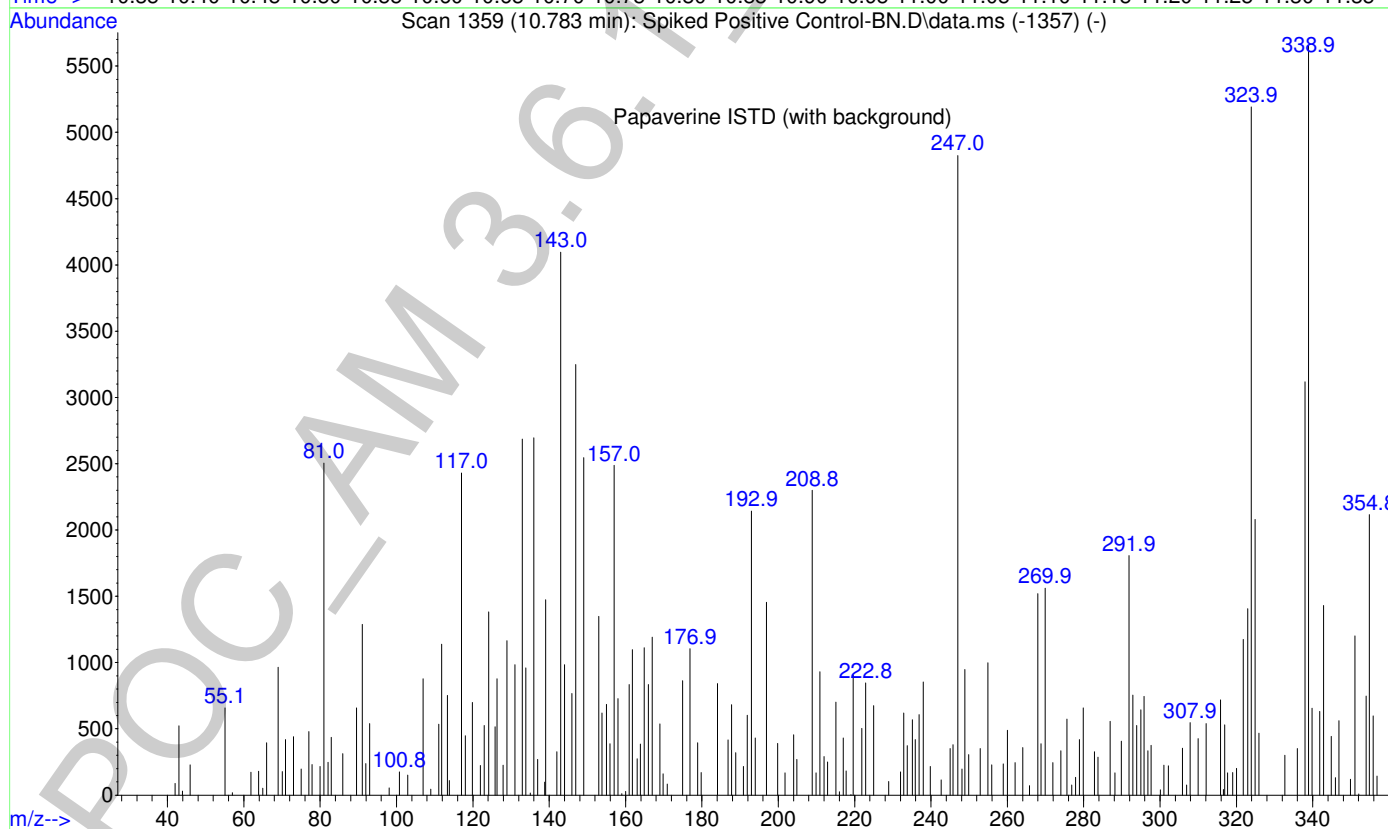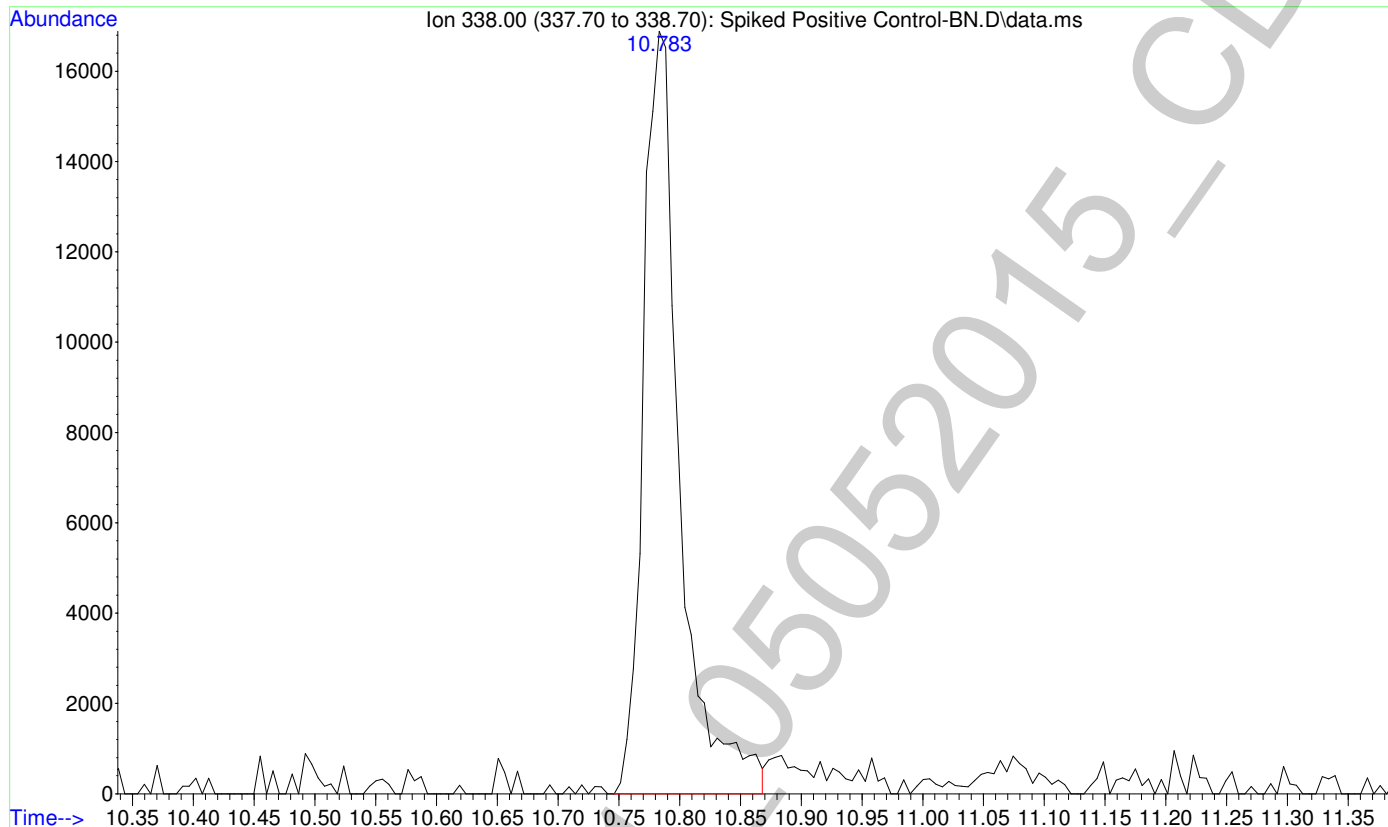



2

File :F:\Data\050515\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 18:39 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

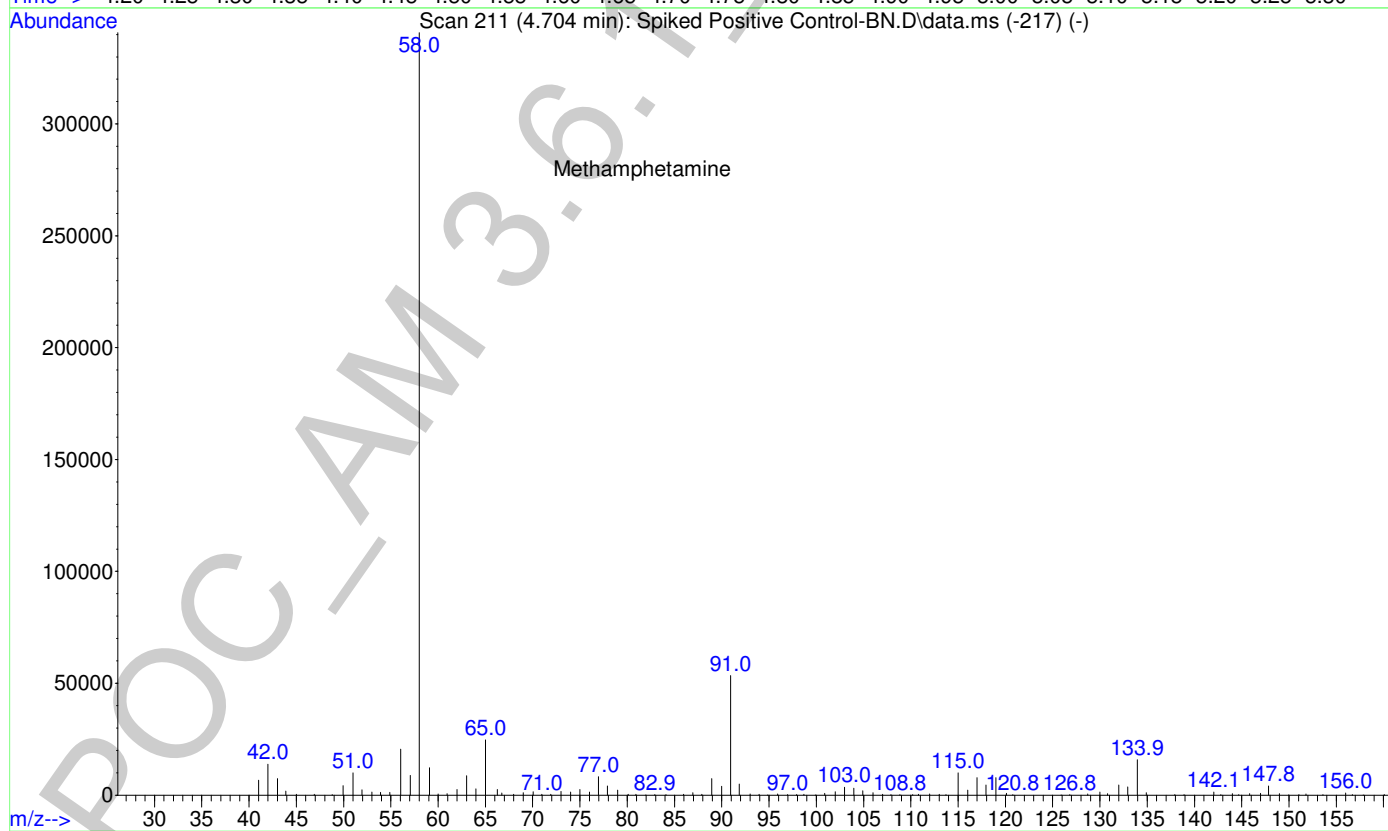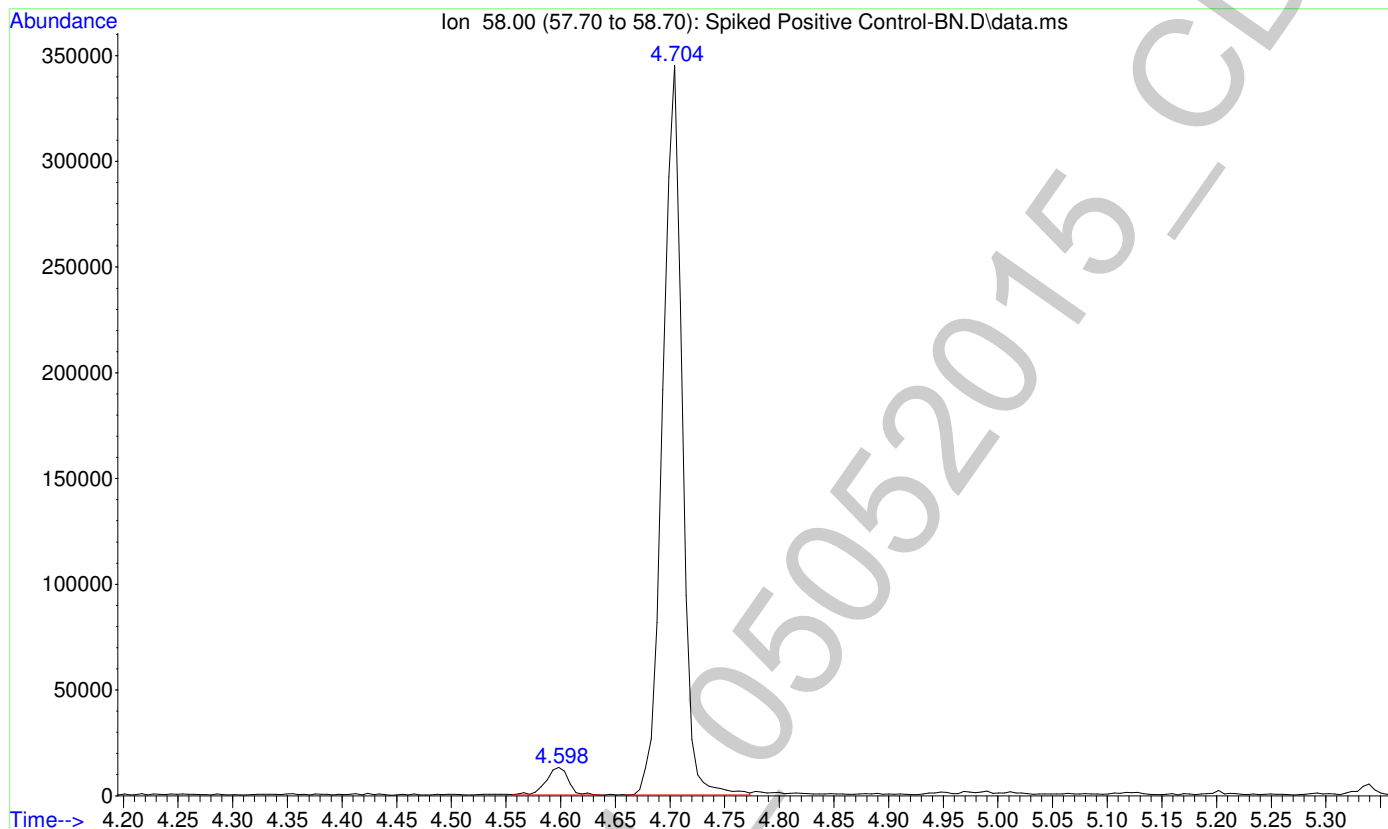



6

File :F:\Data\050515\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 18:39 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

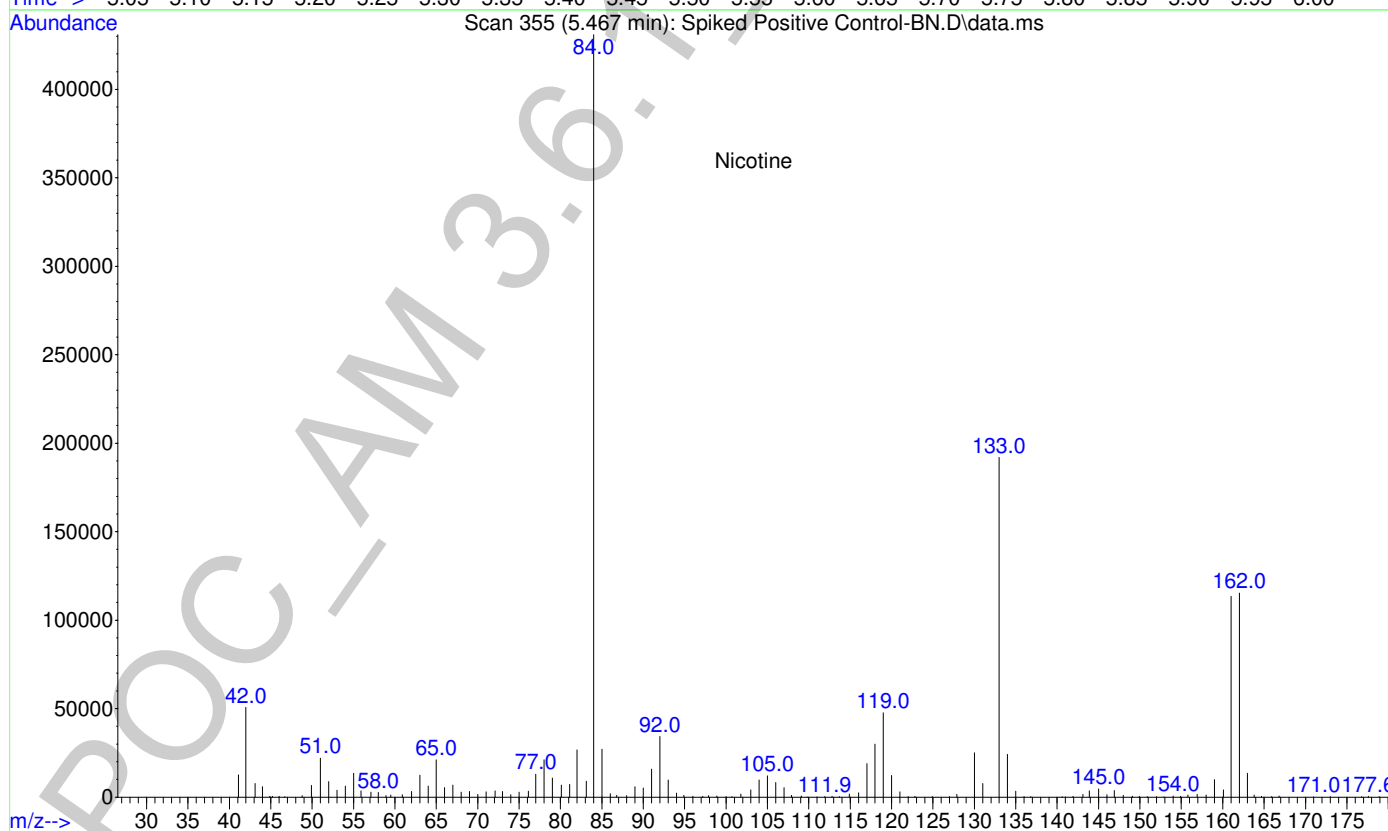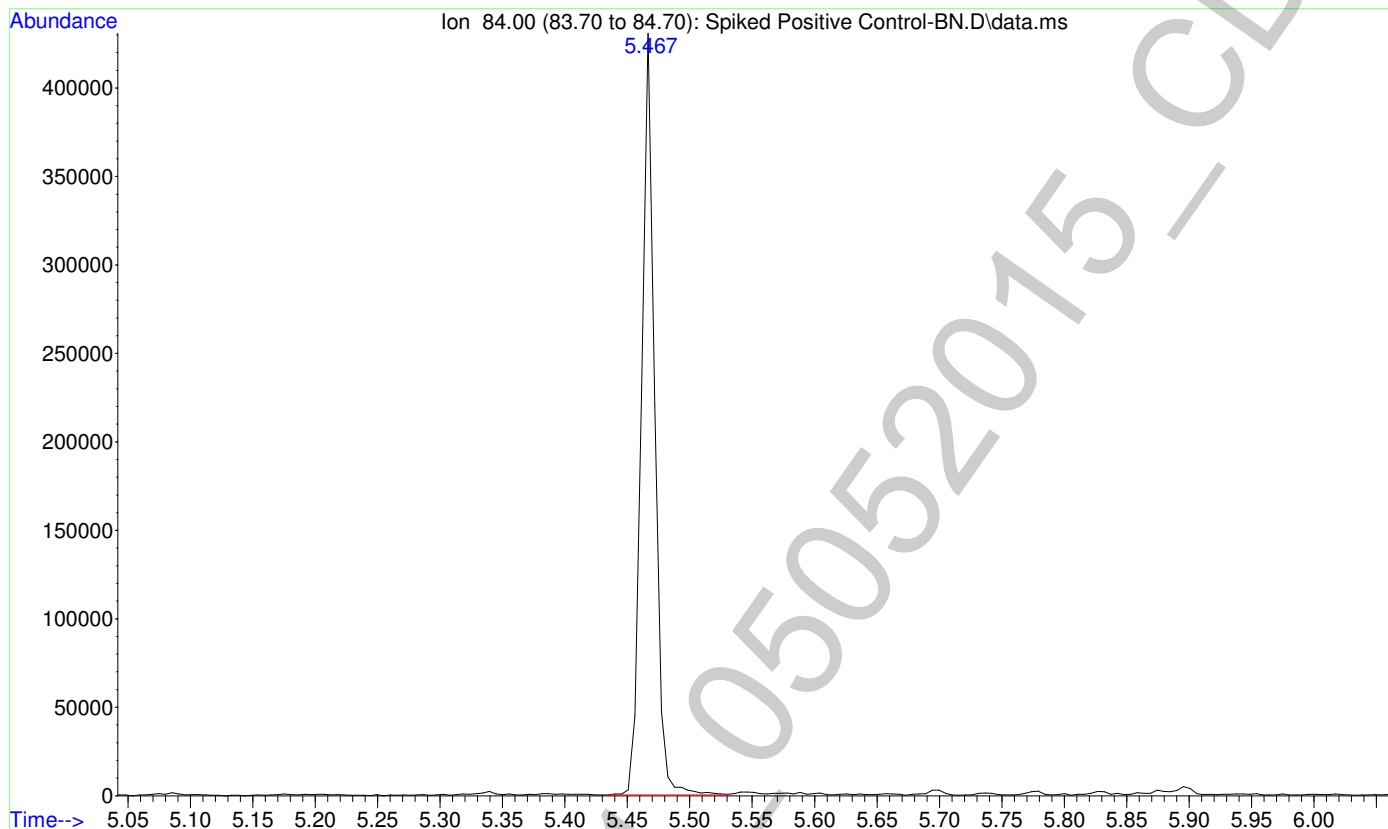



6

File :F:\Data\050515\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 18:39 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

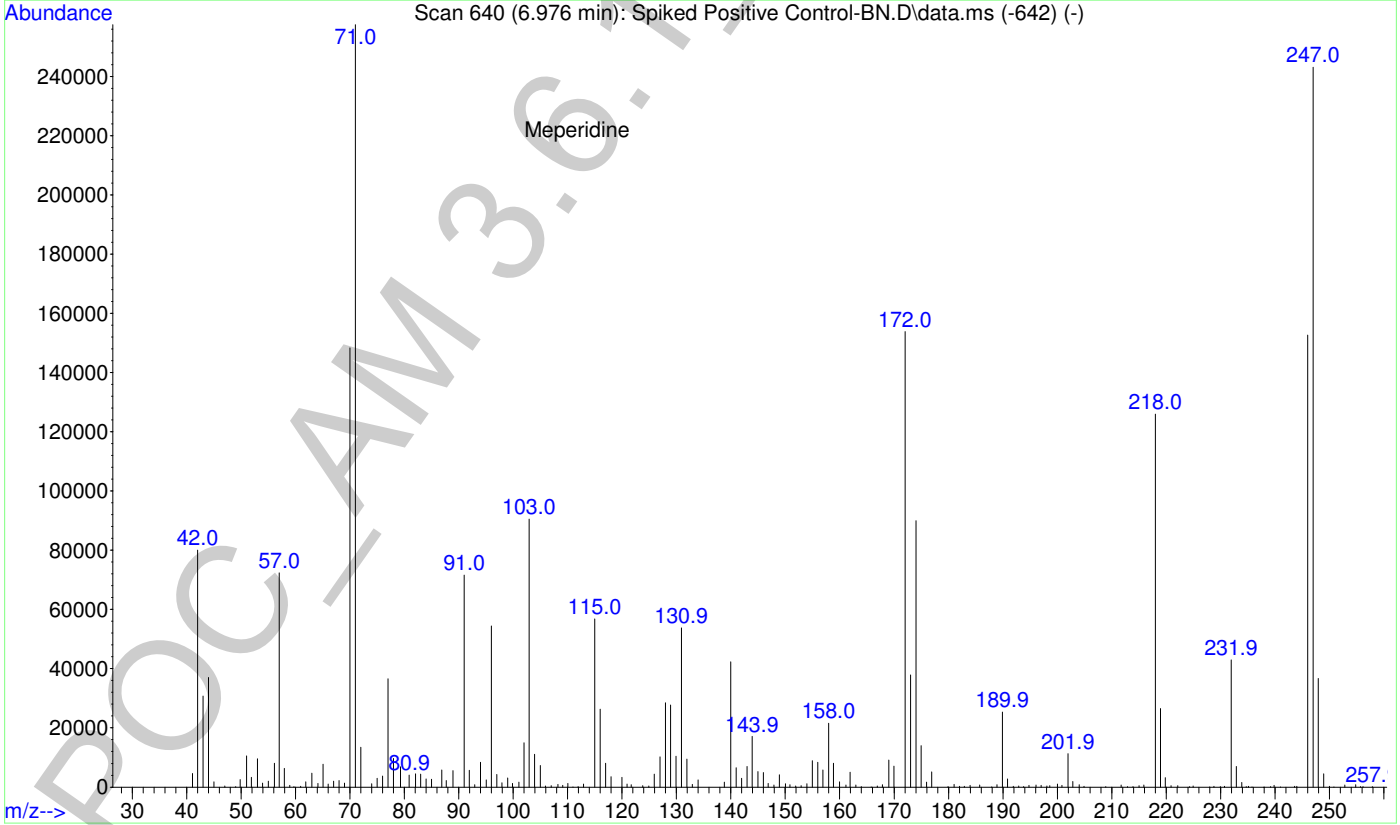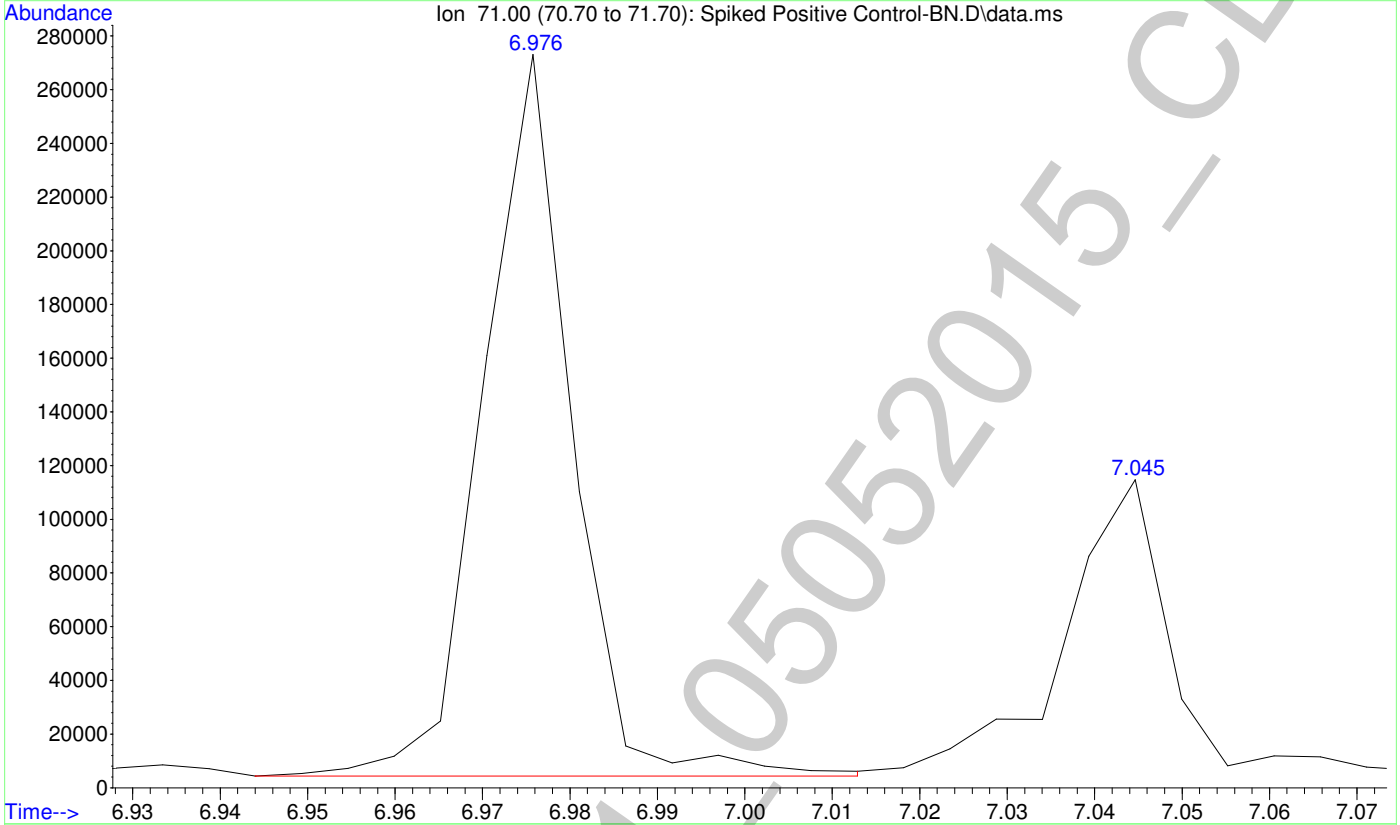



6

File :F:\Data\050515\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 18:39 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

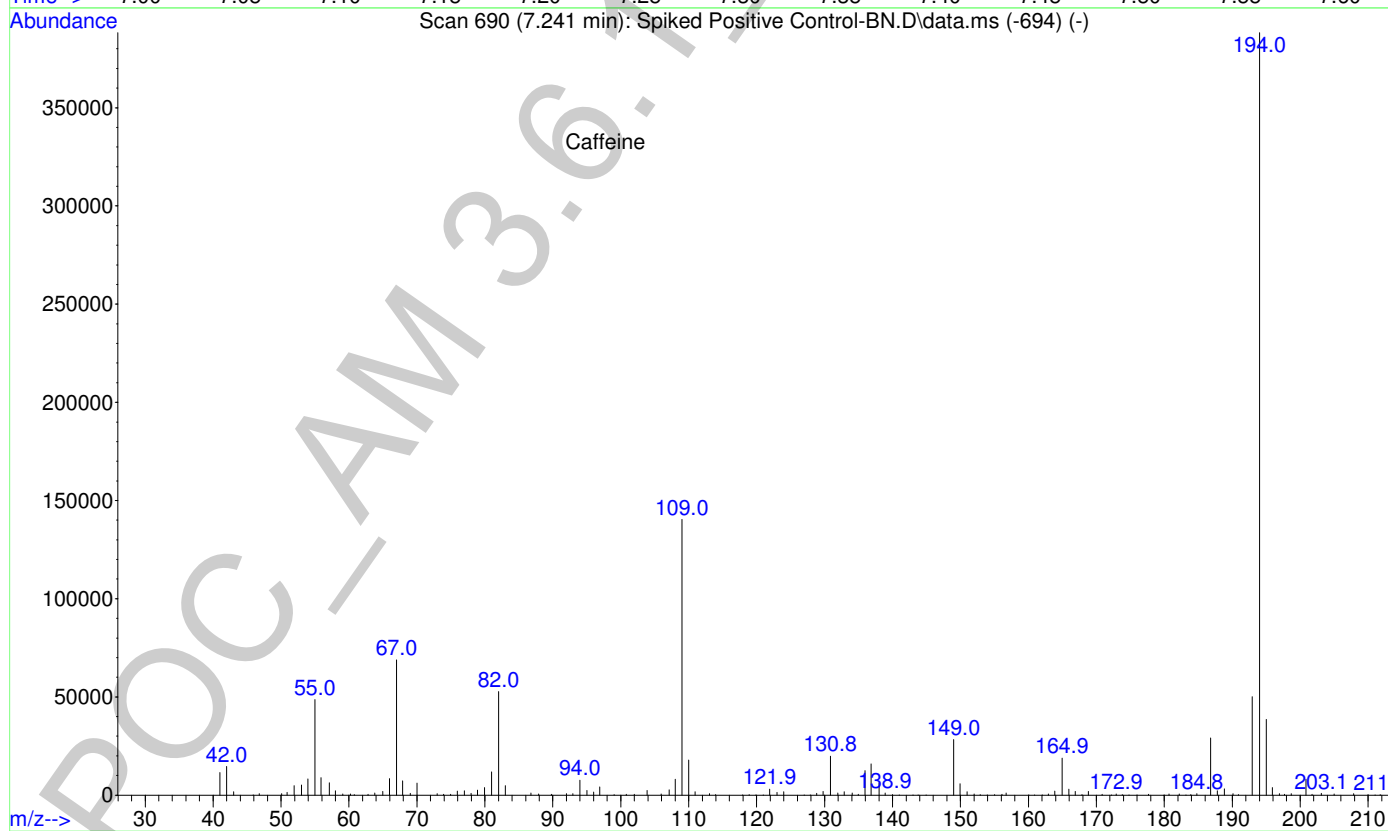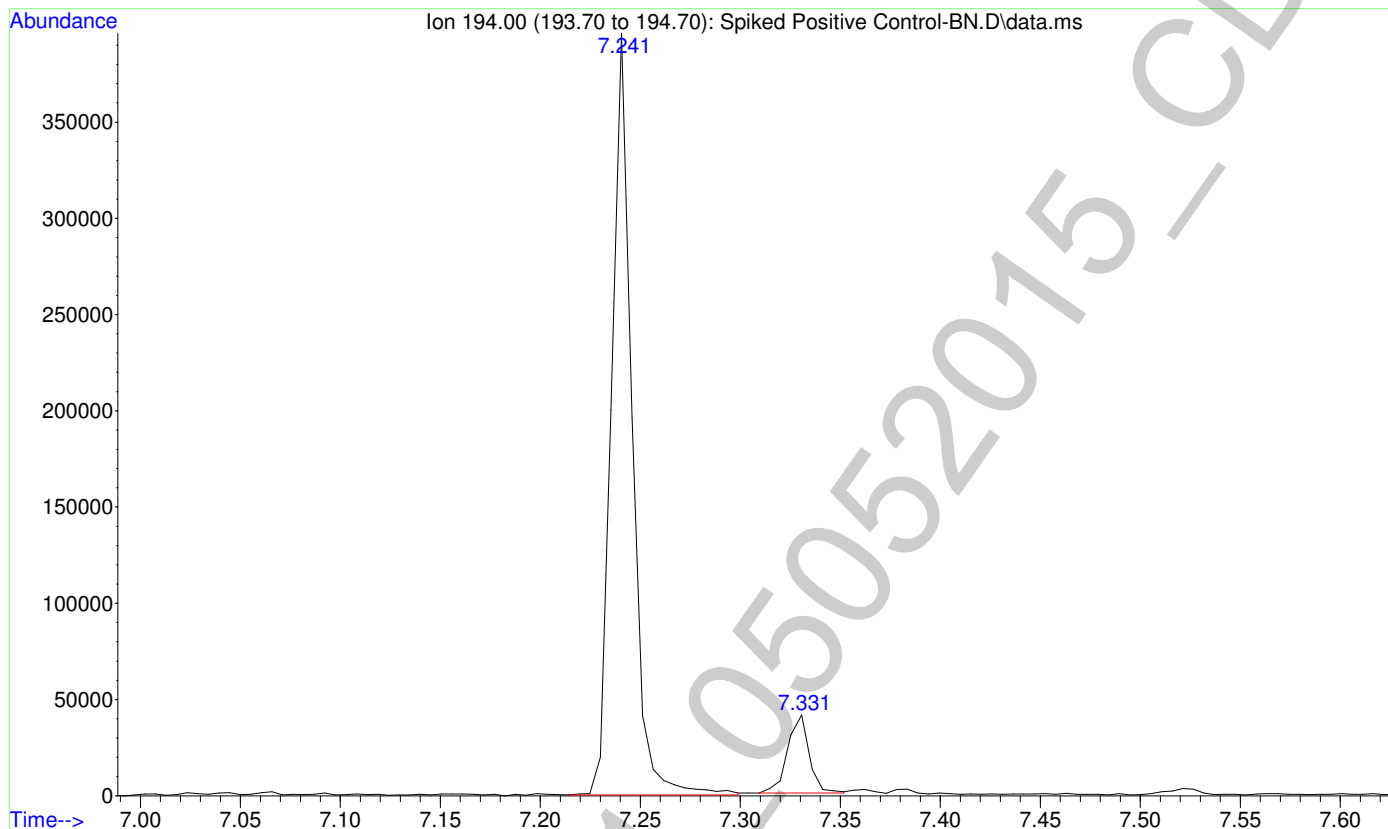



2

File :F:\Data\050515\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 18:39 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

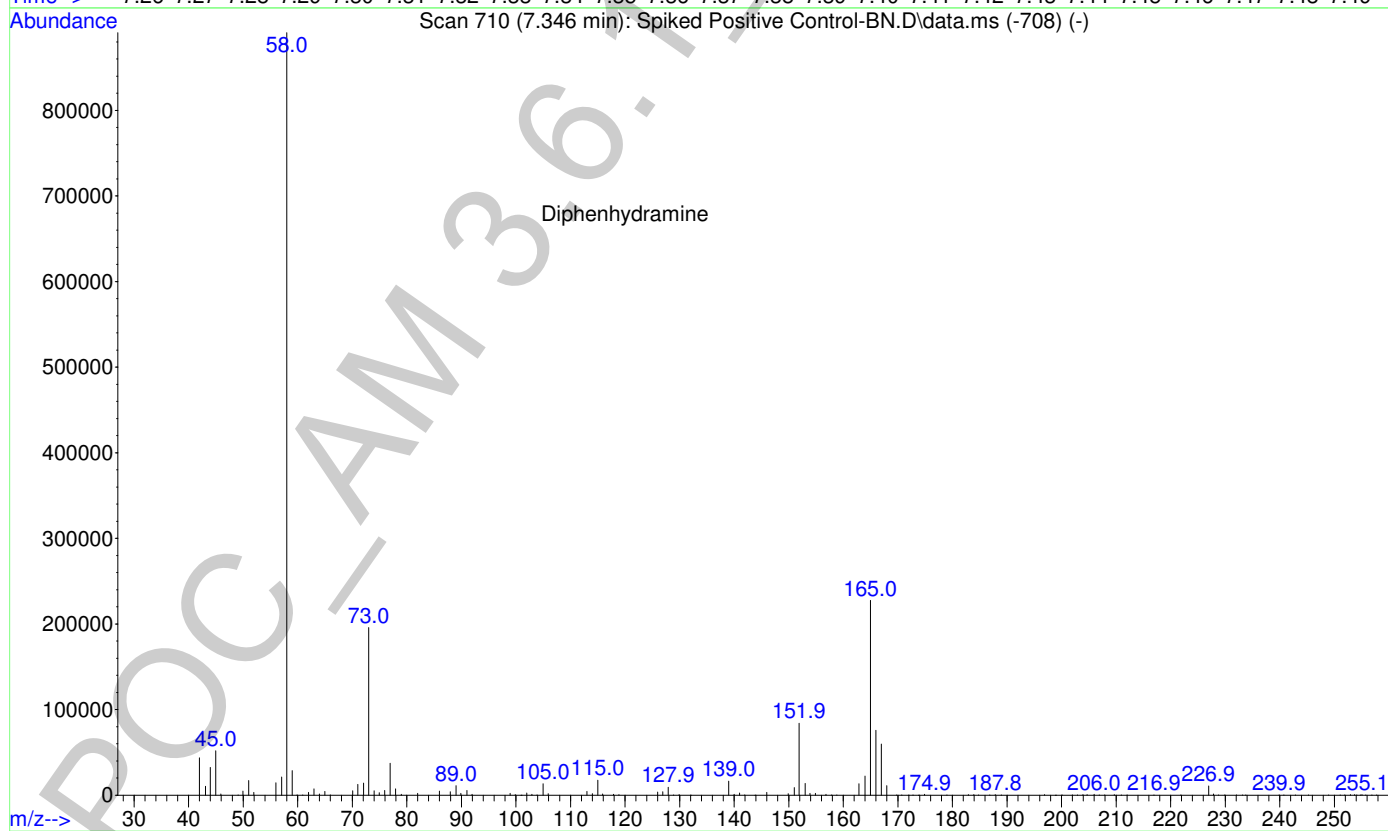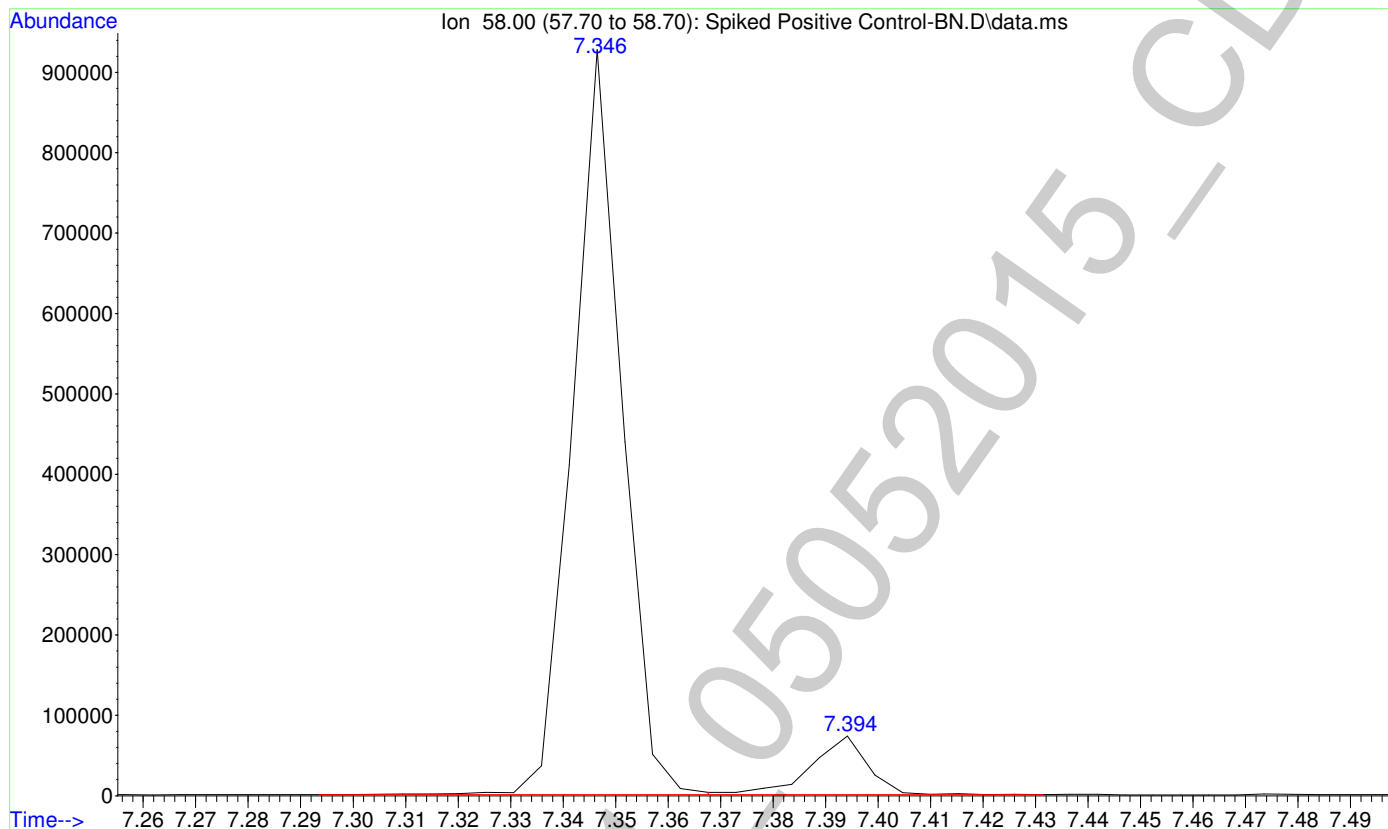



2

File :F:\Data\050515\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 18:39 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

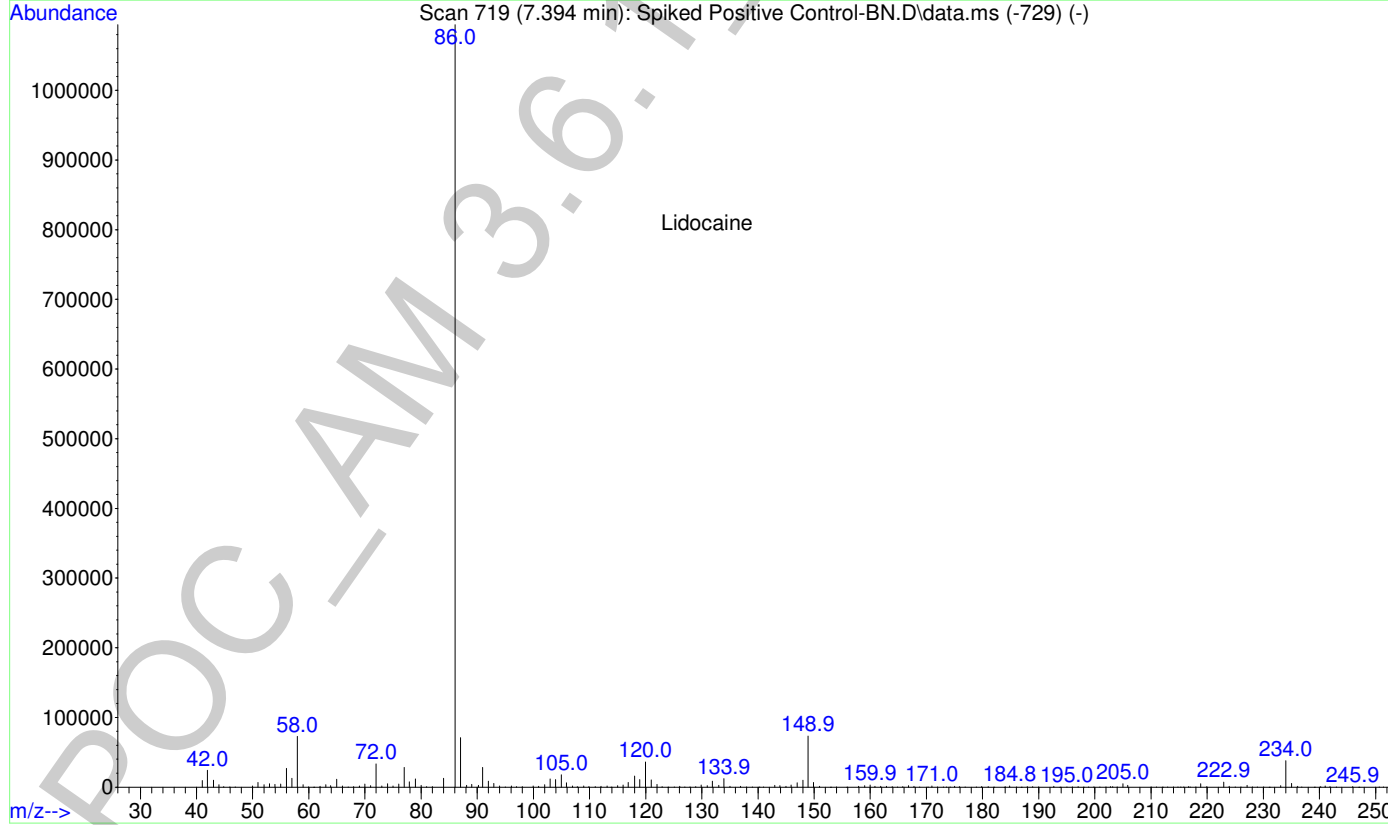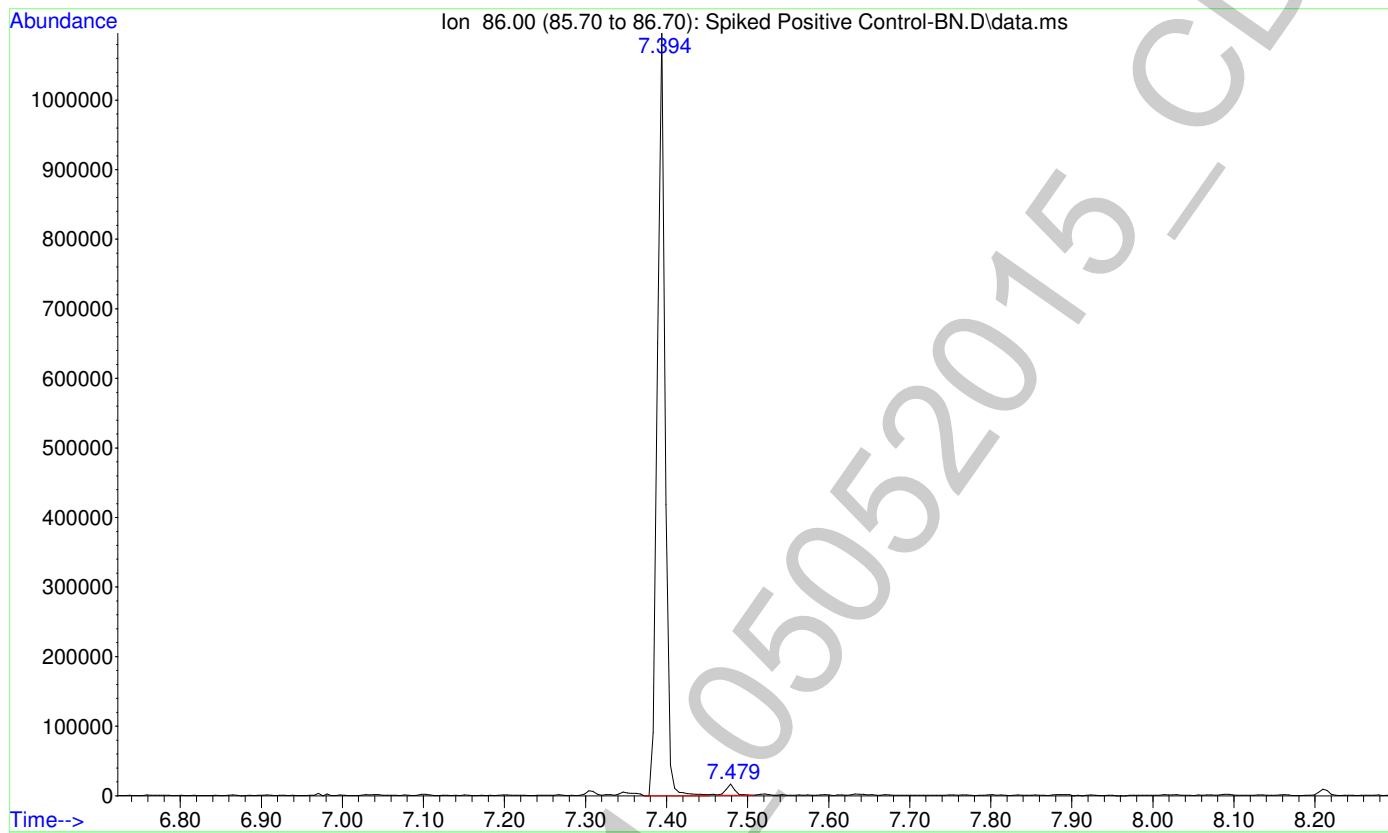



File : F:\Data\050515\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 18:39 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

6

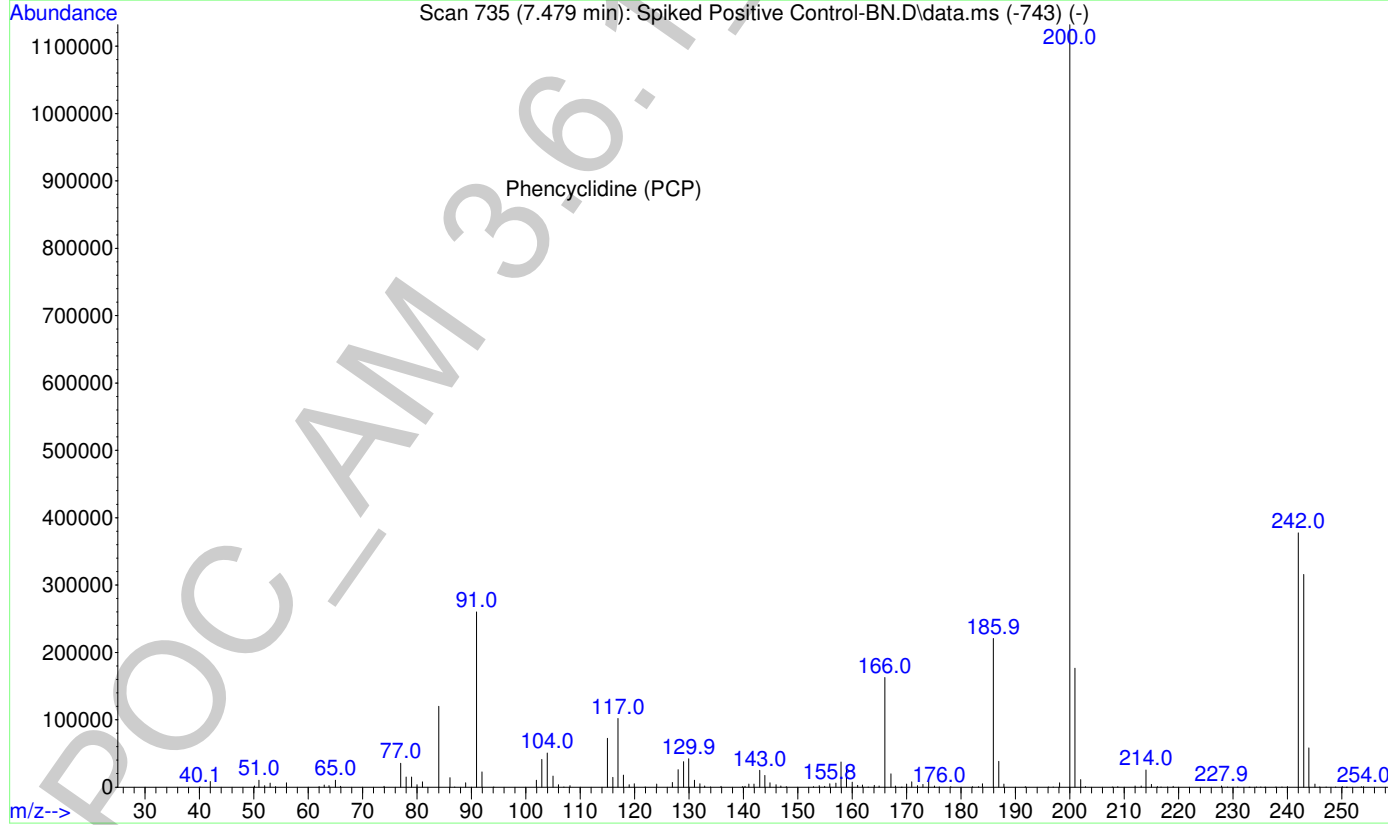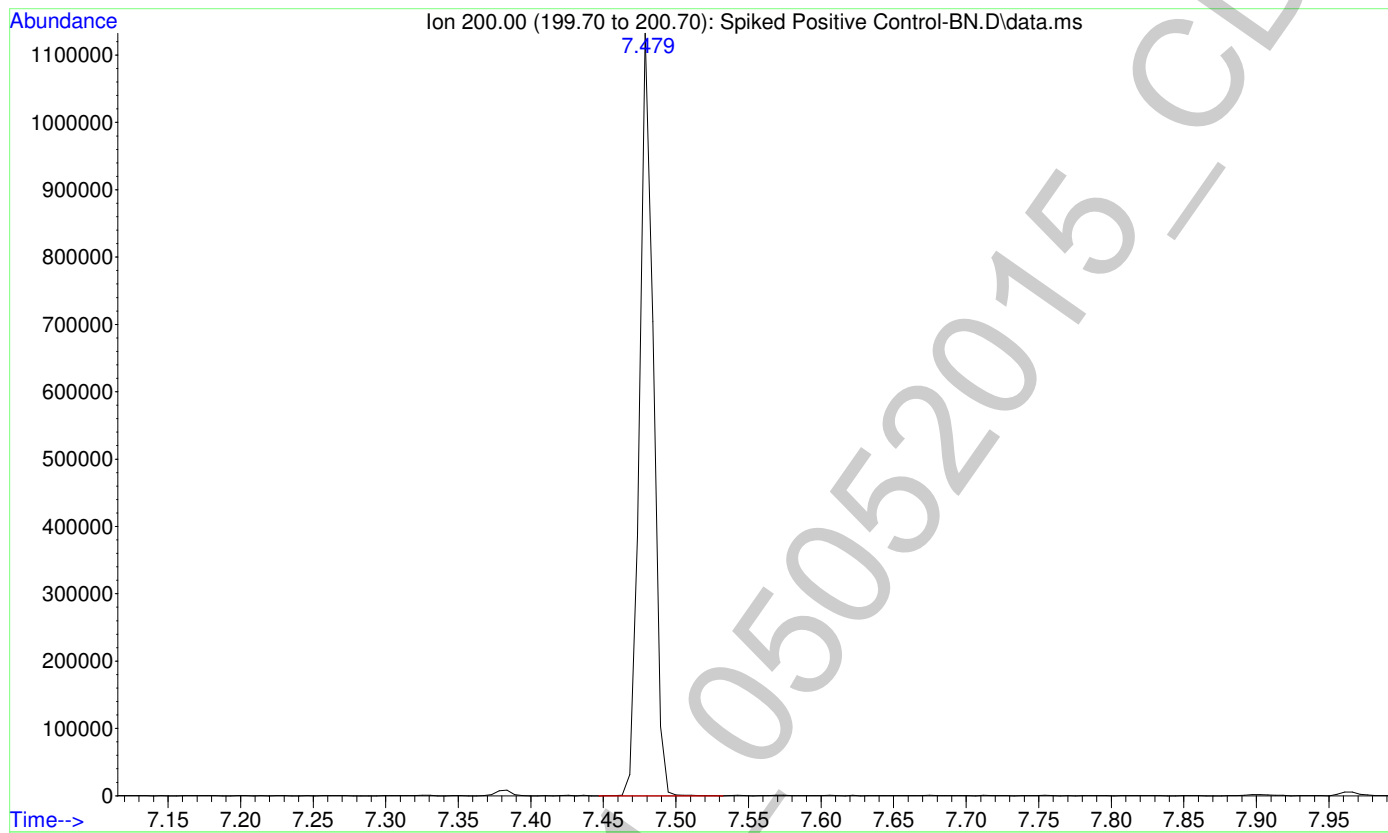



6

File :F:\Data\050515\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 18:39 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

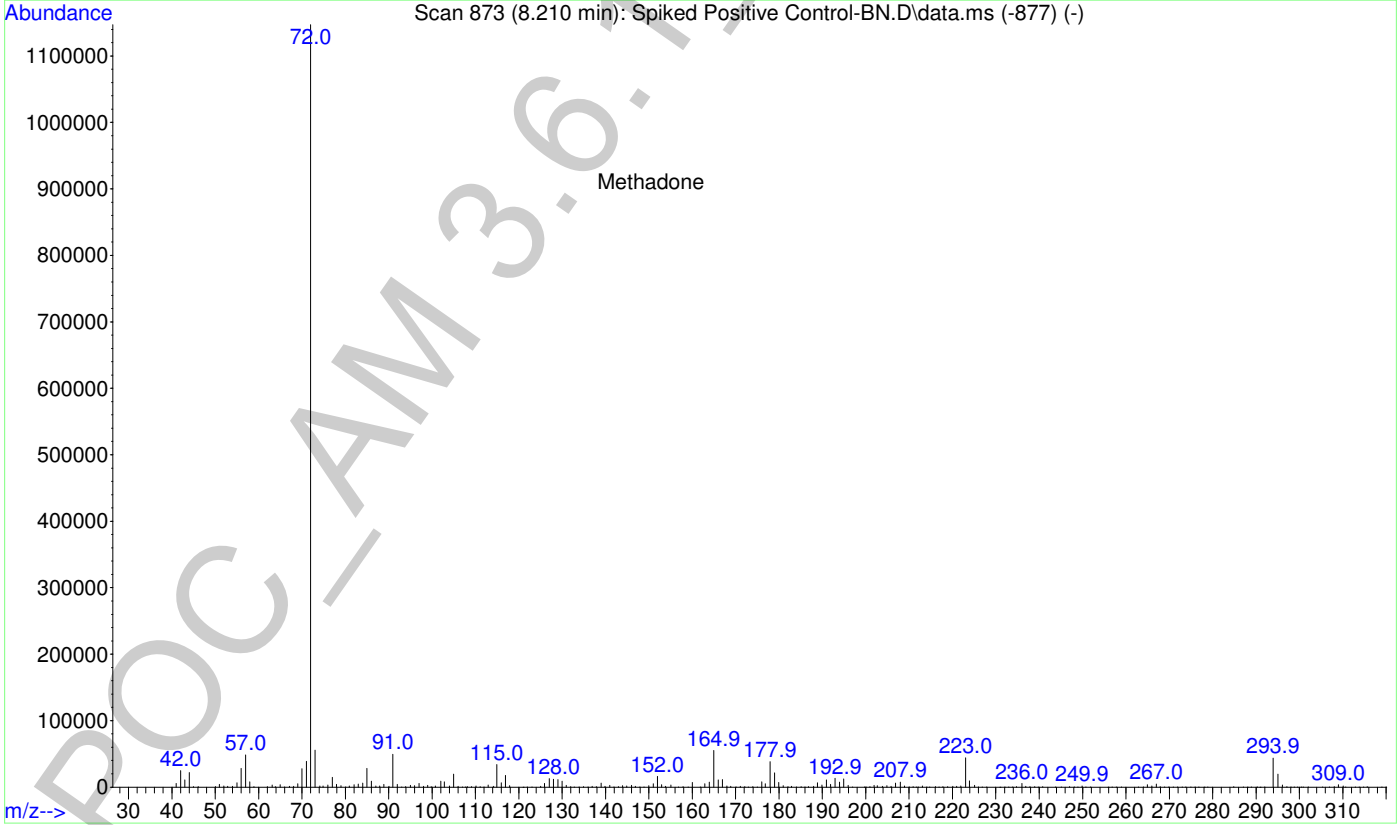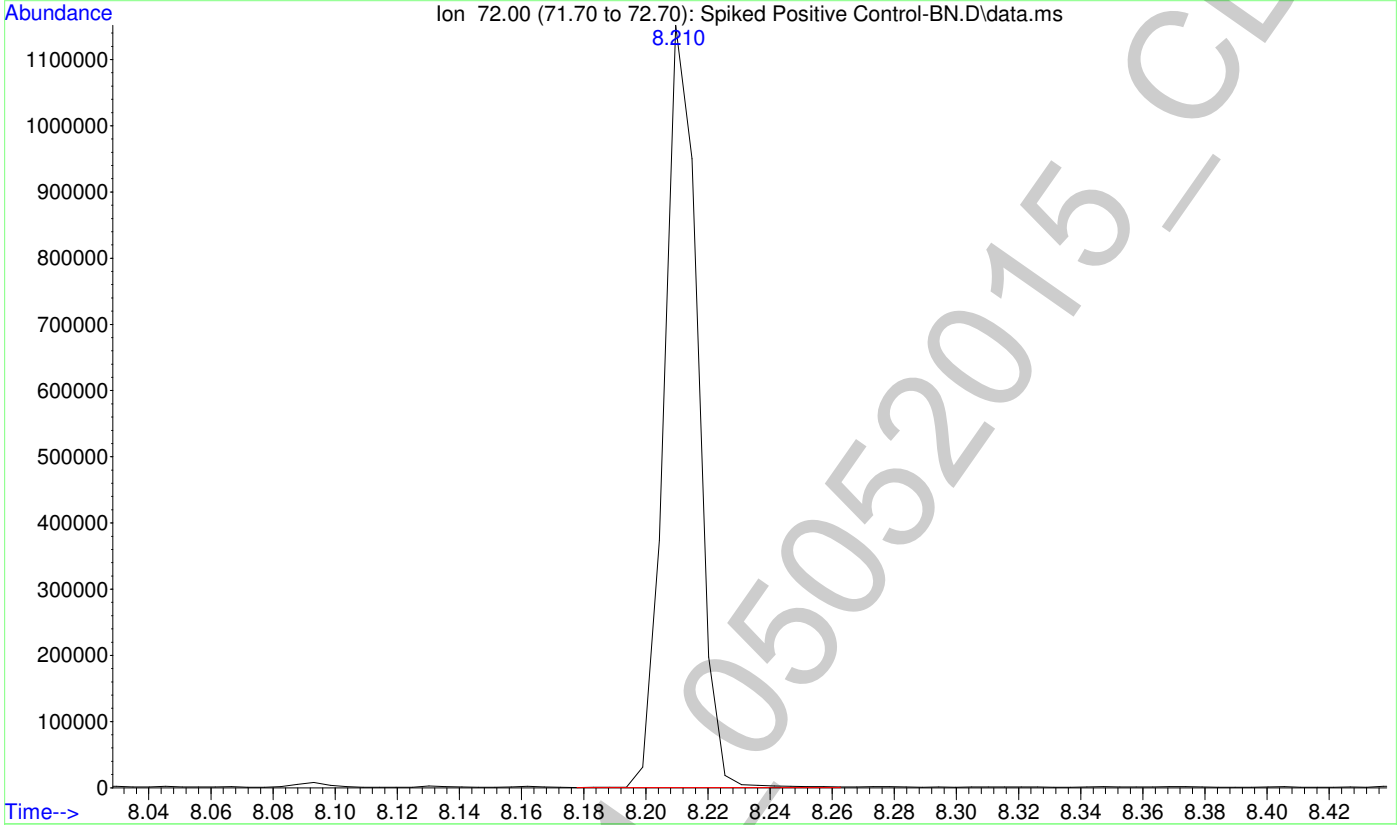



2

File :F:\Data\050515\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 18:39 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

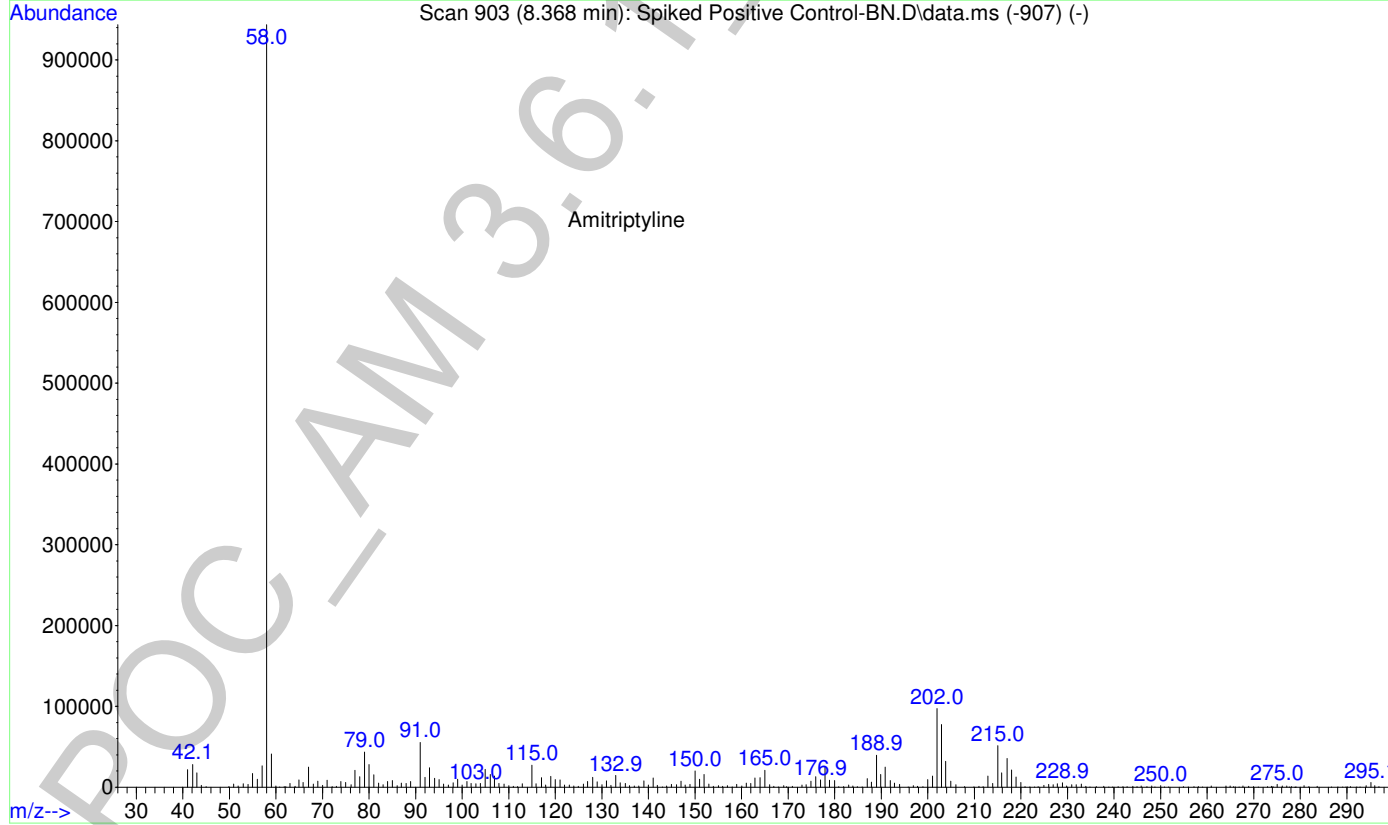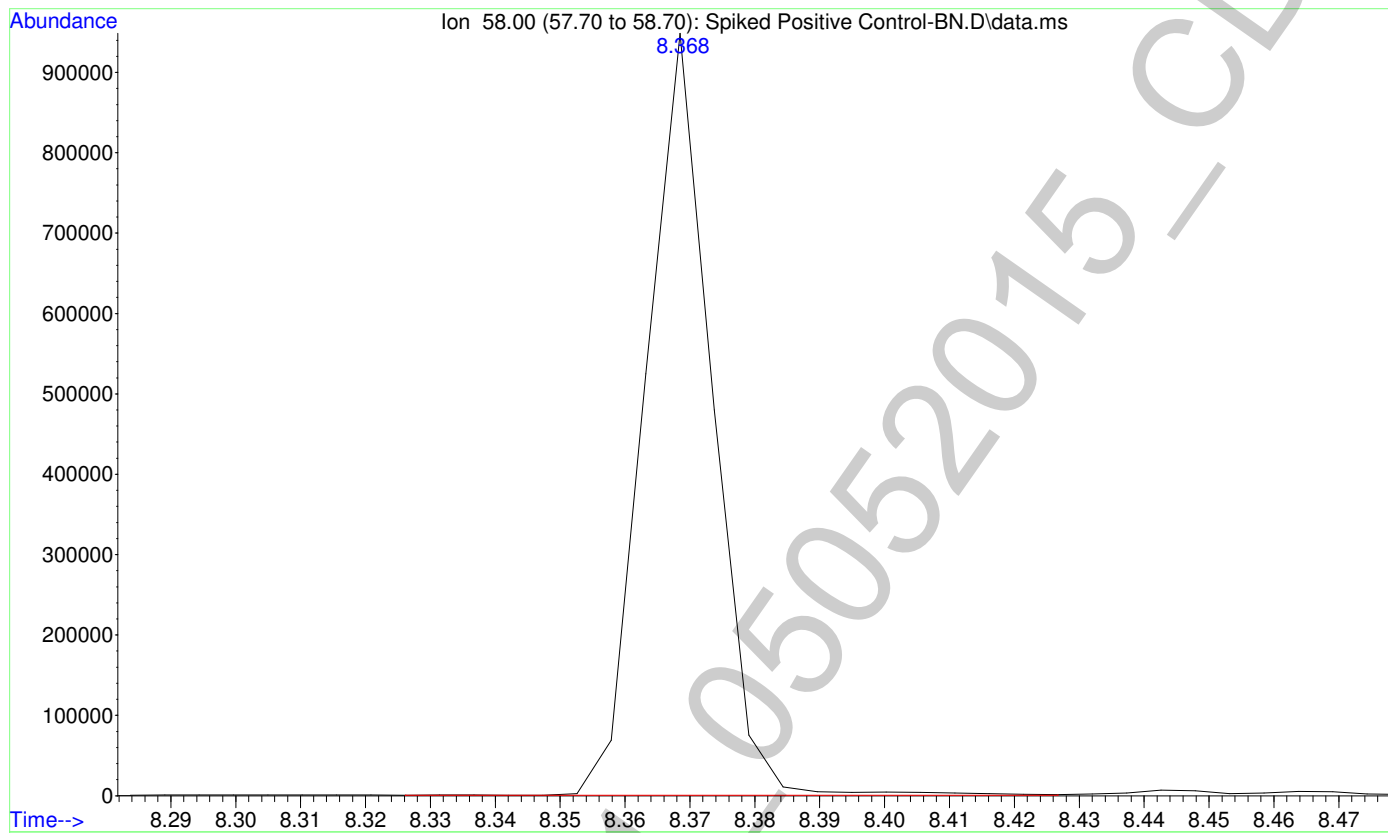



2

File :F:\Data\050515\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 18:39 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

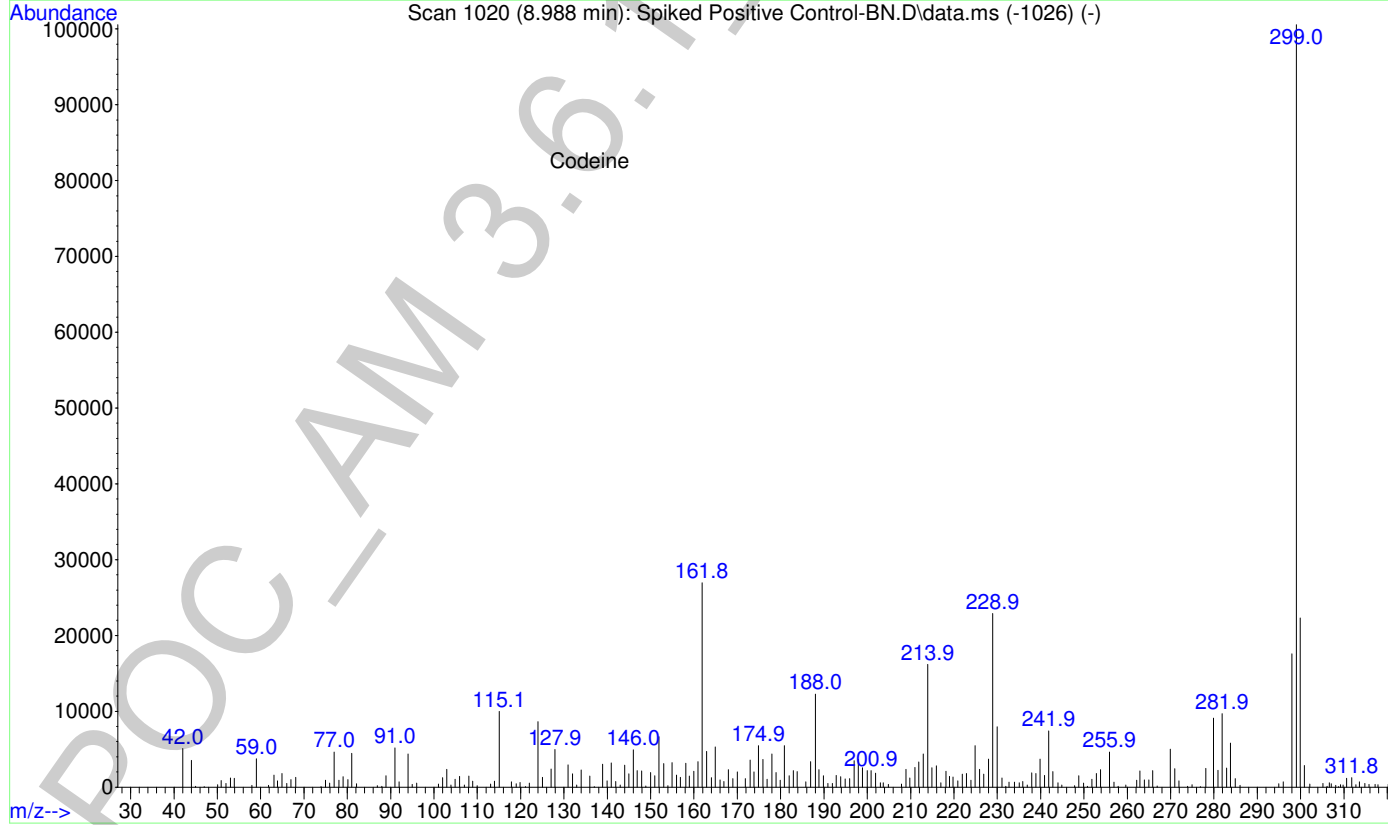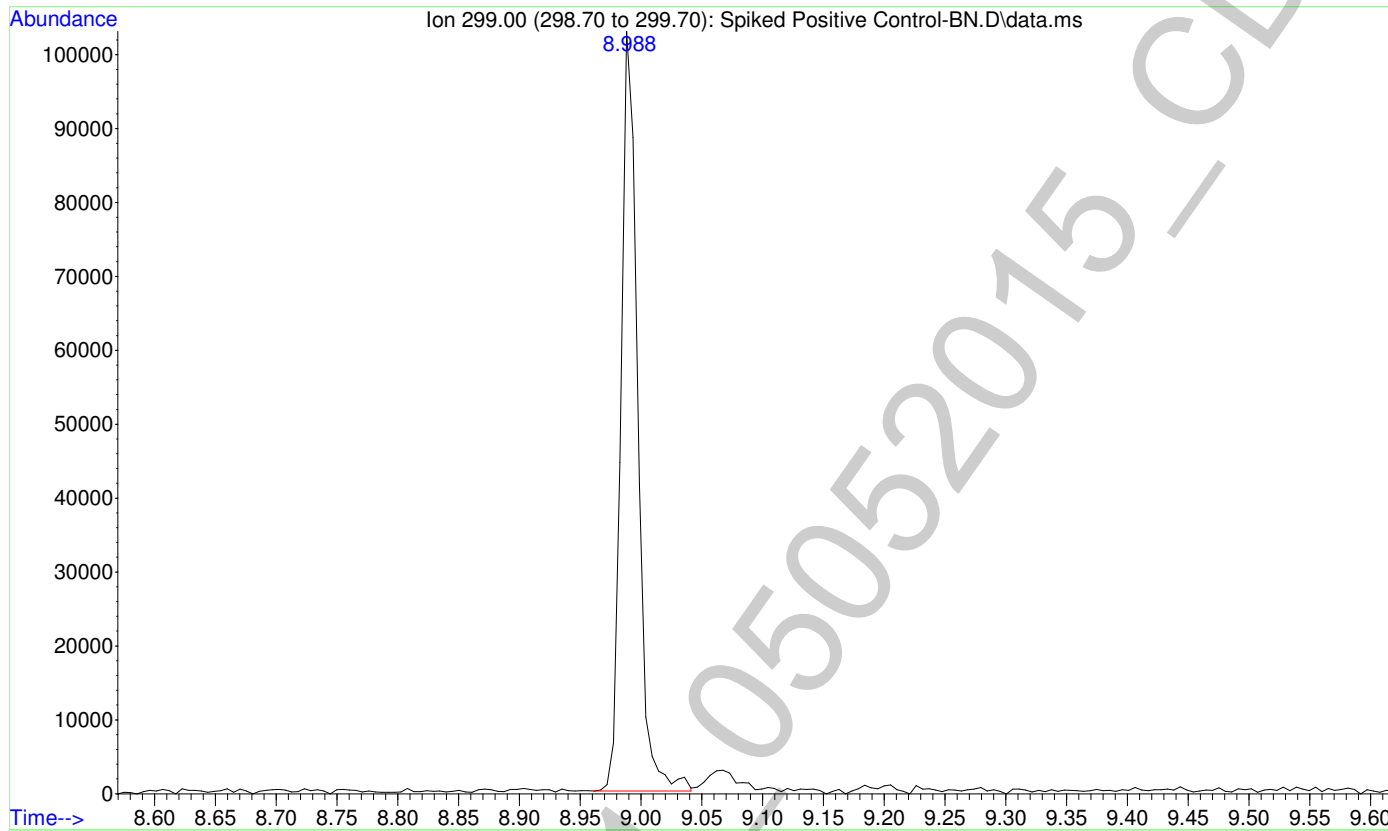

File :F:\Data\050515\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 18:39 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

2

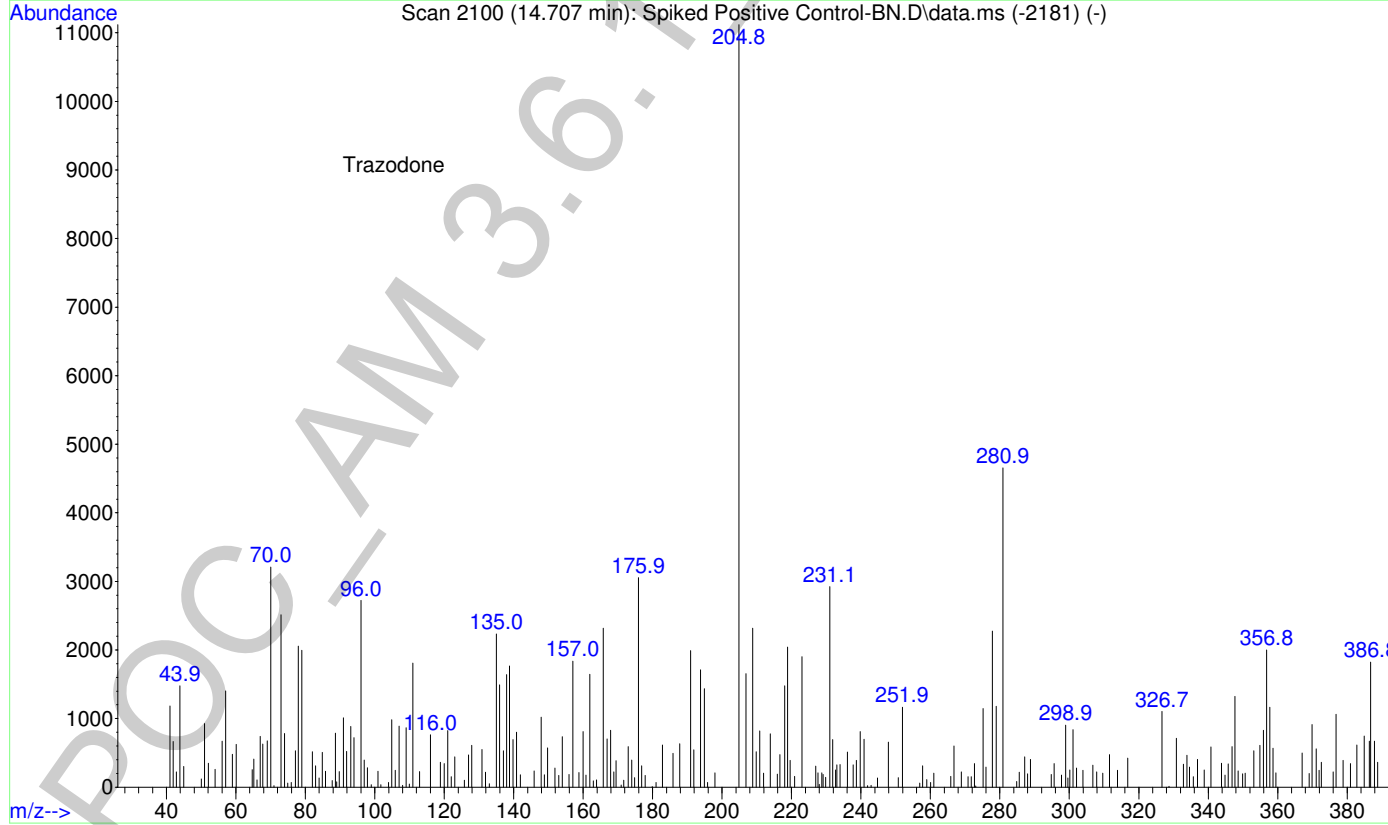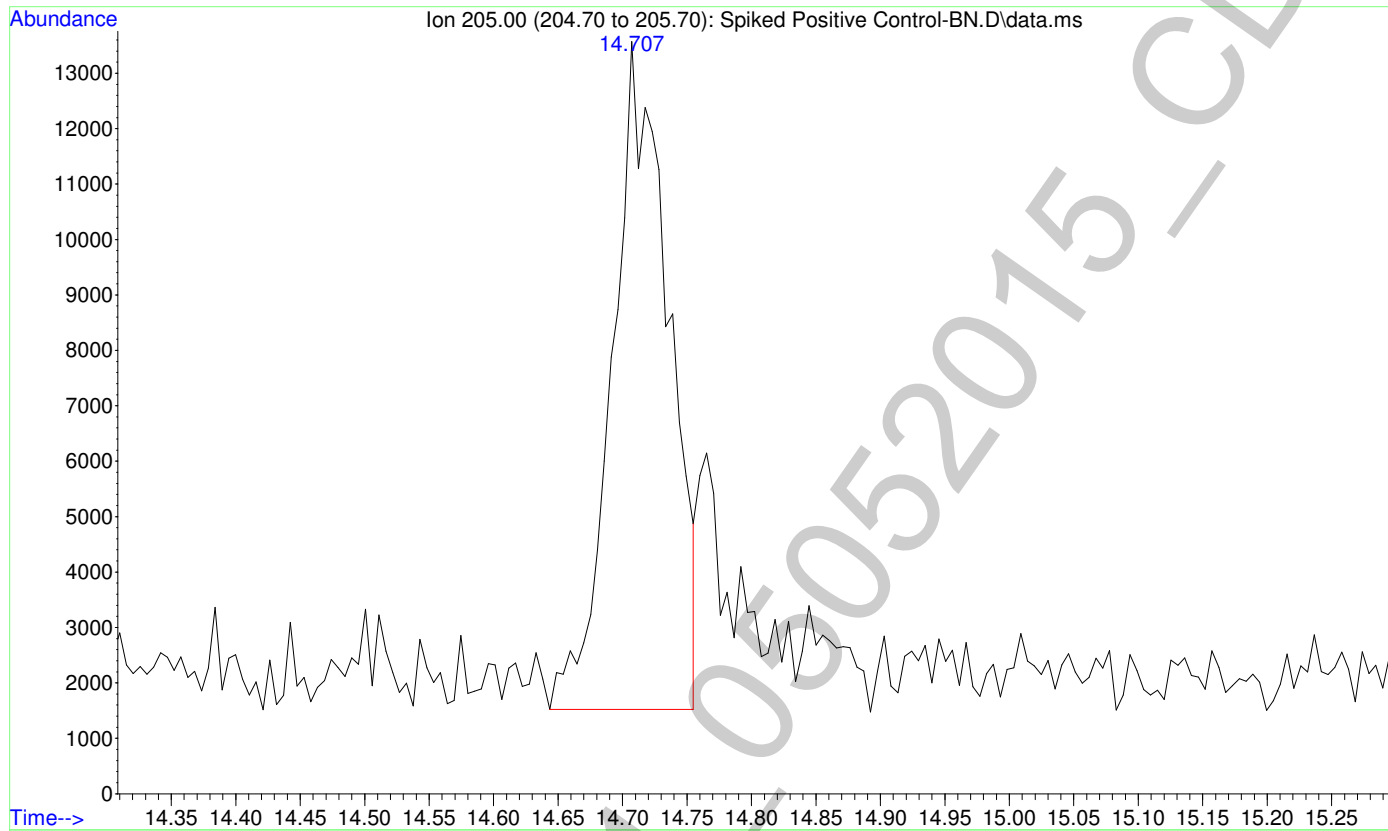

6

Analytical Method 3.6.1 & 3.6.7 QA Check List

Run Start Date: 05/05/15

Analyst: CS

(Long GC/MS temperature program)

Positive Control Compound List

- Methamphetamine
- Nicotine
- Meperidine
- Caffeine
- Diphenhydramine
- Lidocaine
- PCP
- Methadone
- Amitriptyline
- Codeine
- Trazodone

Internal Standards



- Benzphetamine
- Papaverine

Optional back extraction **not** performed.
Reconstituted in MeOH.

POC_AM3.6.1_05052015_CDS



2

File :F:\Data\050515\Prerun Solvent Blankr.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 19:25 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Pre-run Solvent Blank
Misc Info : Chloroform
Vial Number: 100

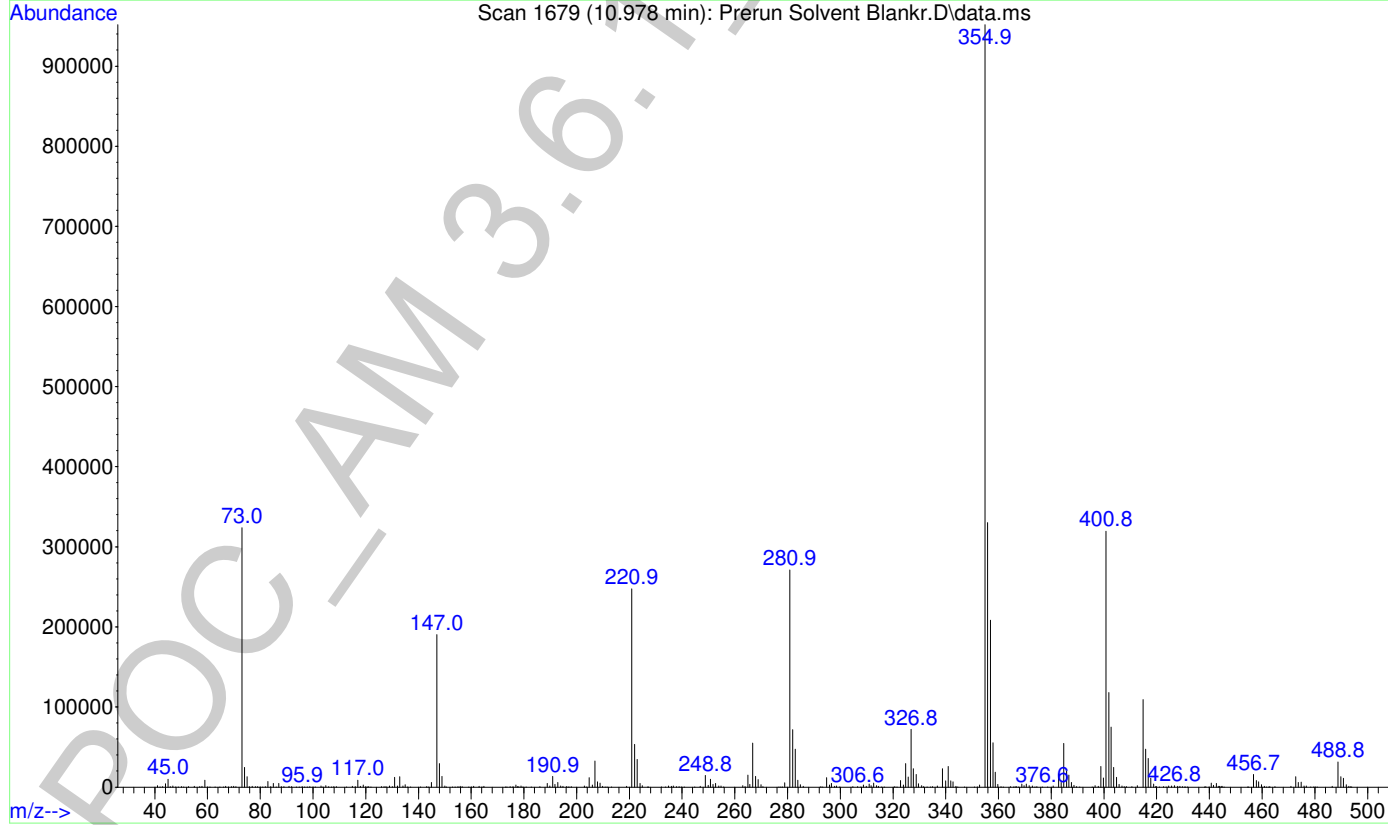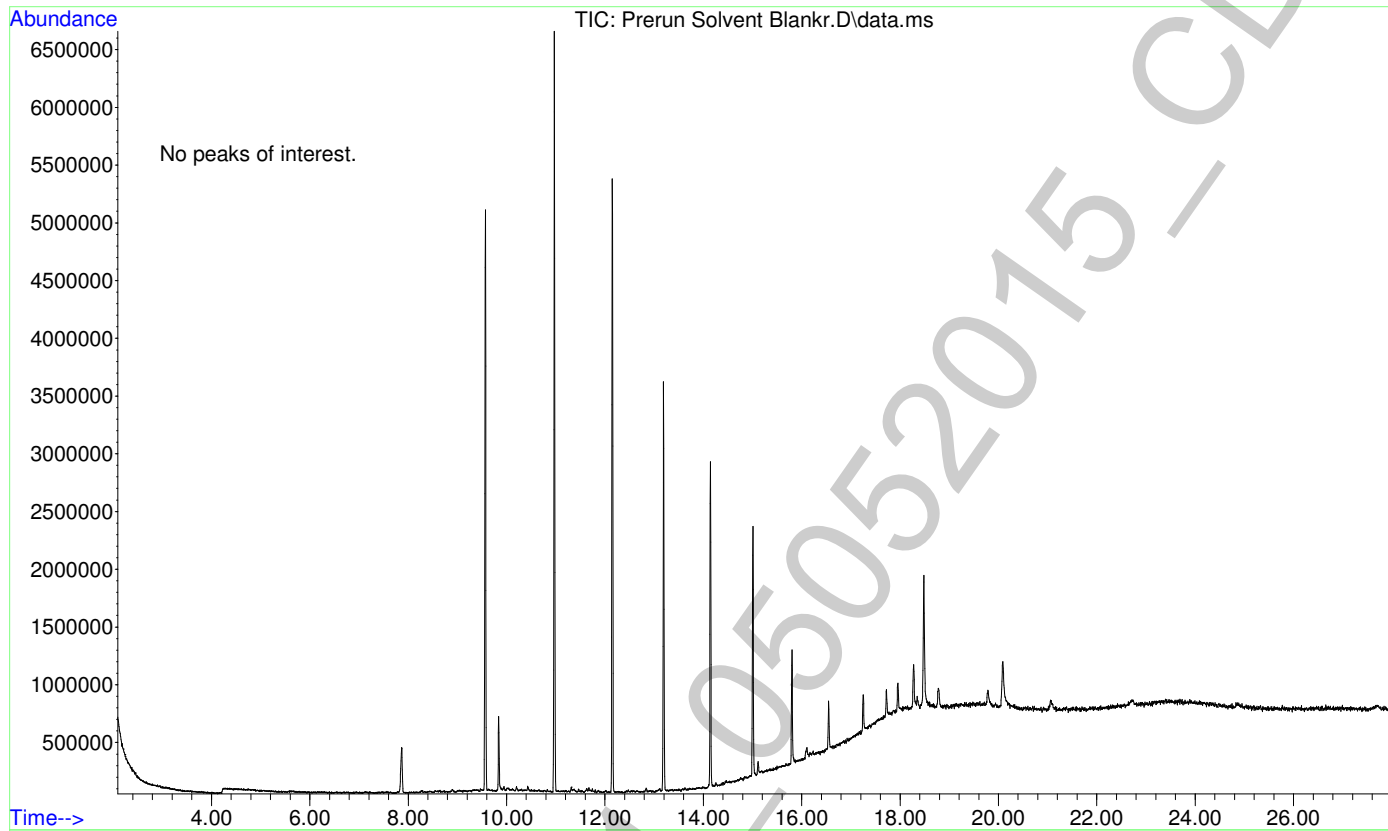


File :F:\Data\050515\prbLK2r.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 21:07 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Solvent Blank
Misc Info : Chloroform
Vial Number: 99

2

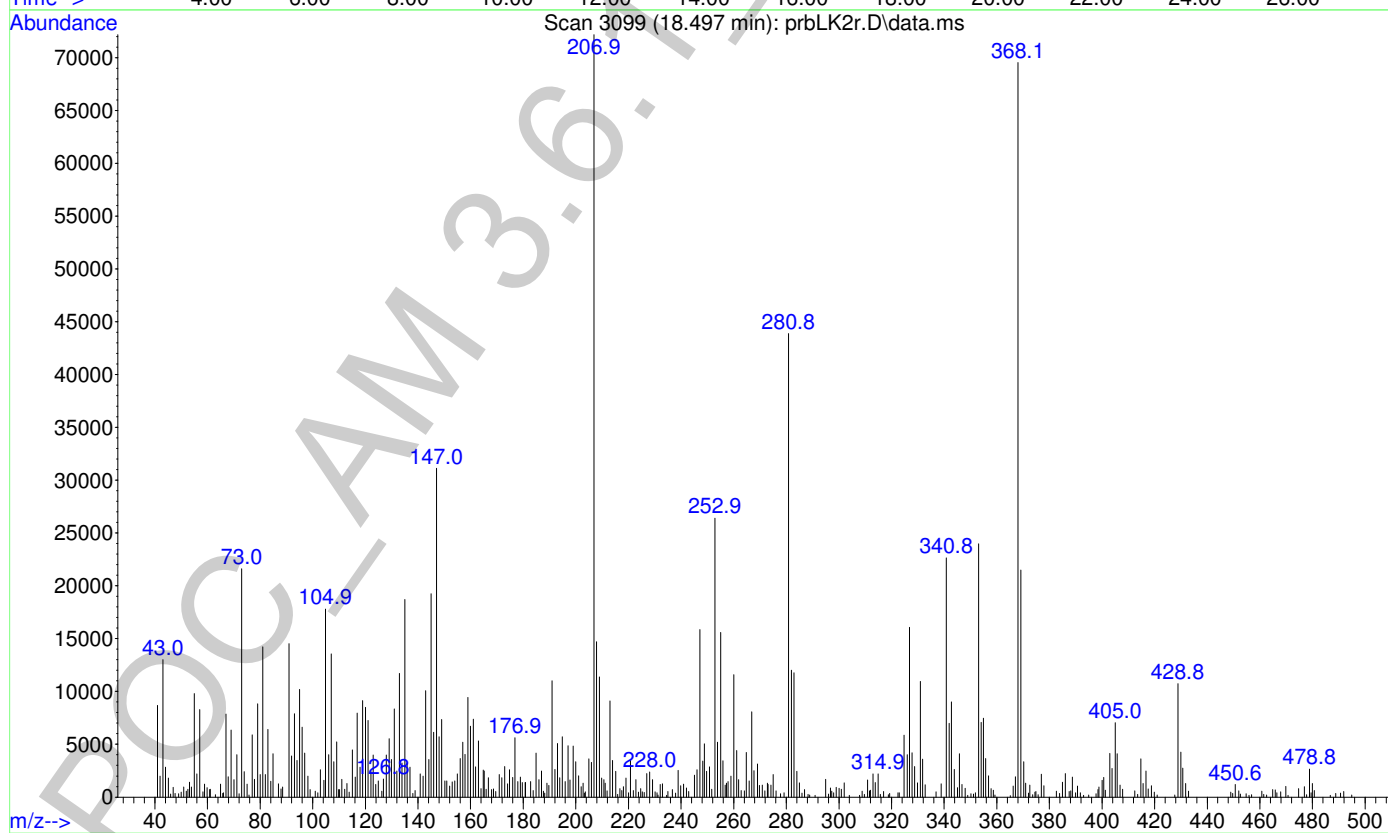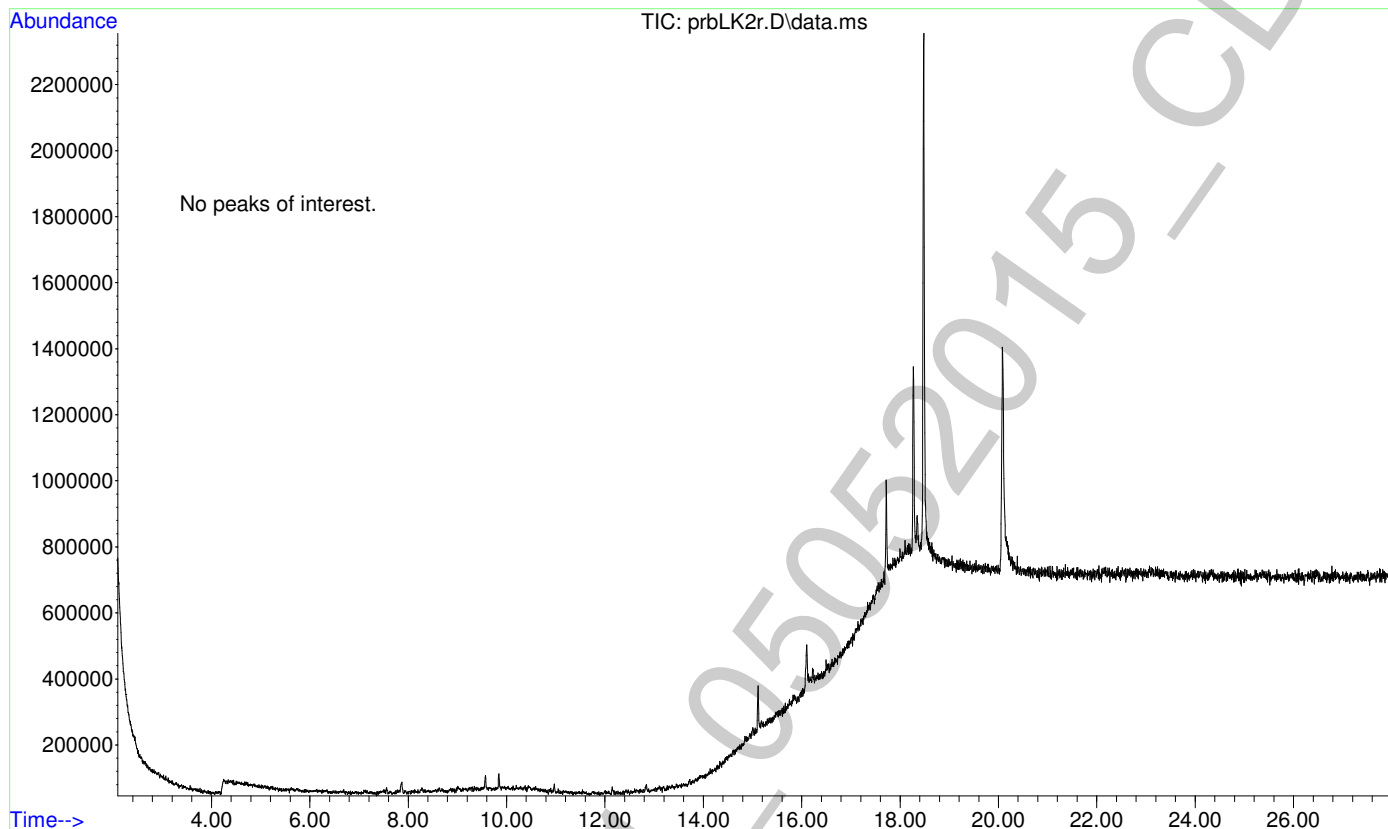



2

File :F:\Data\050515\Negative Control-BNr.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 19:59 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1
Vial Number: 1

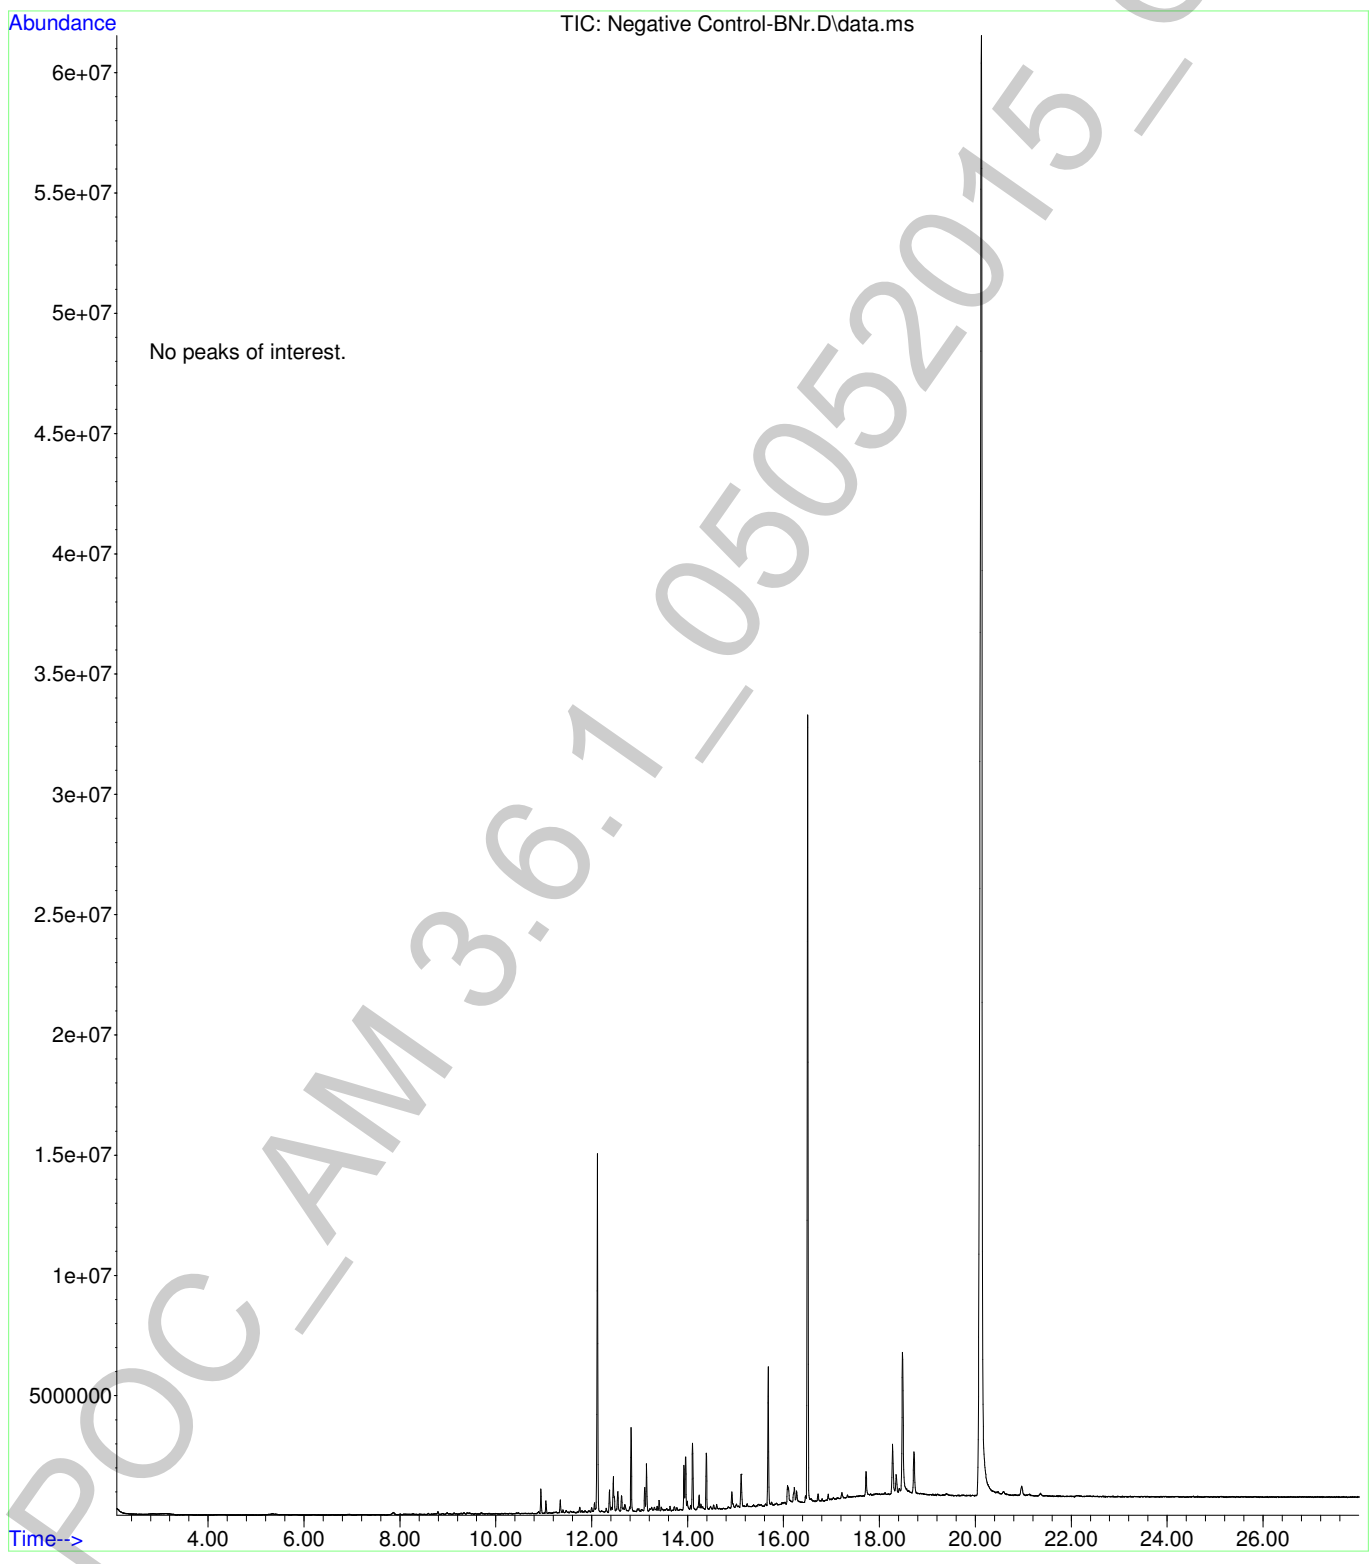



6

File :F:\Data\050515\Negative Control-BNr.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 19:59 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1
Vial Number: 1

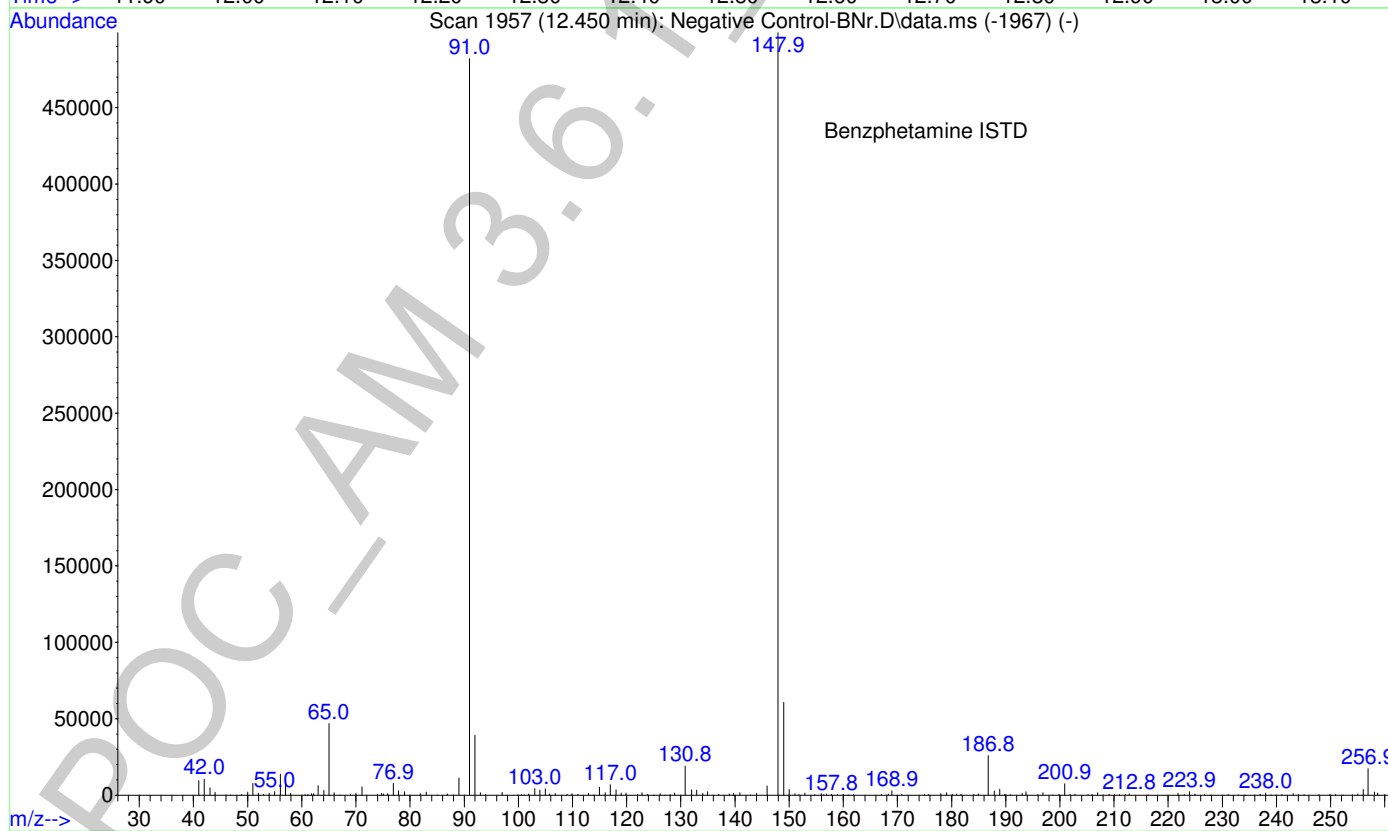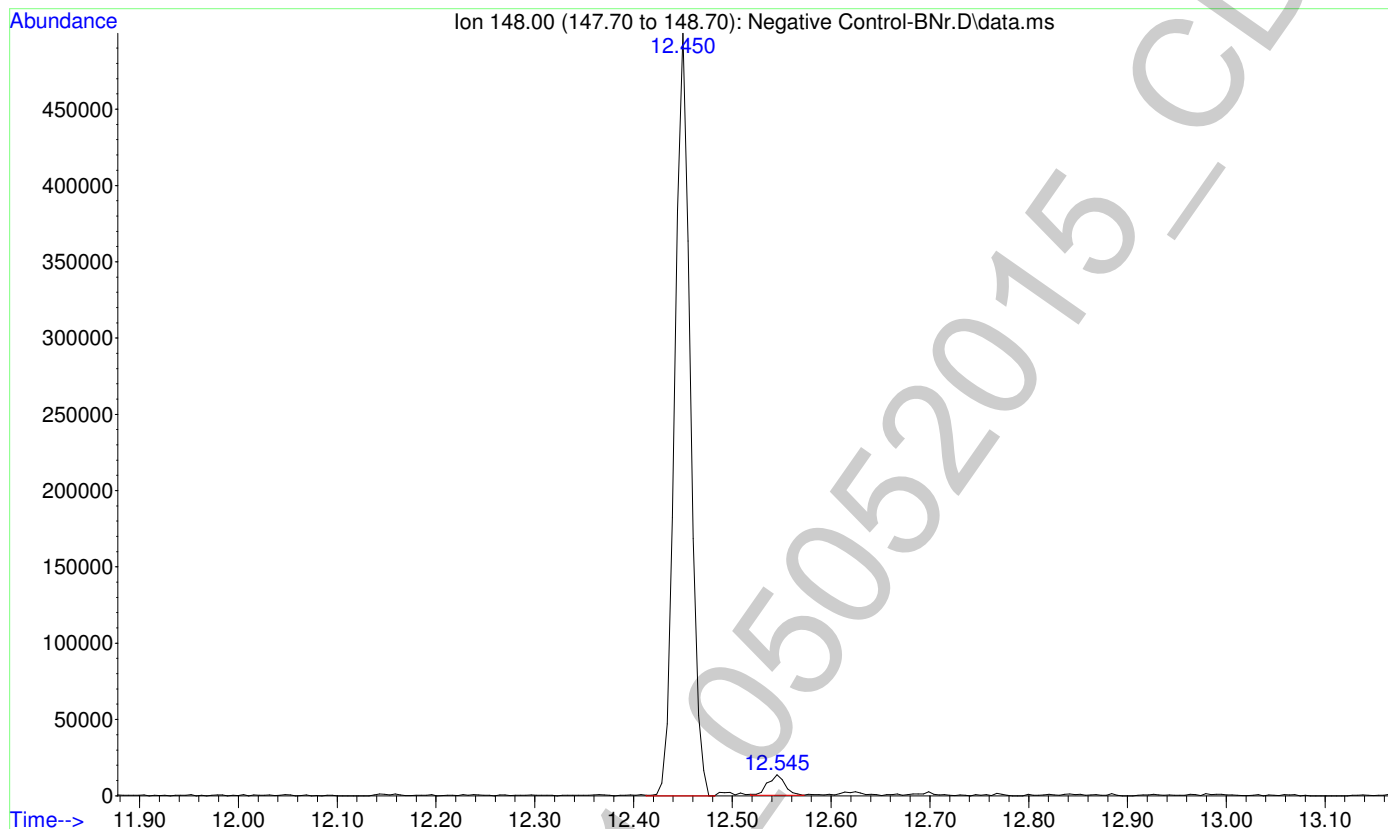


2

File :F:\Data\050515\Negative Control-BNr.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 19:59 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1
Vial Number: 1

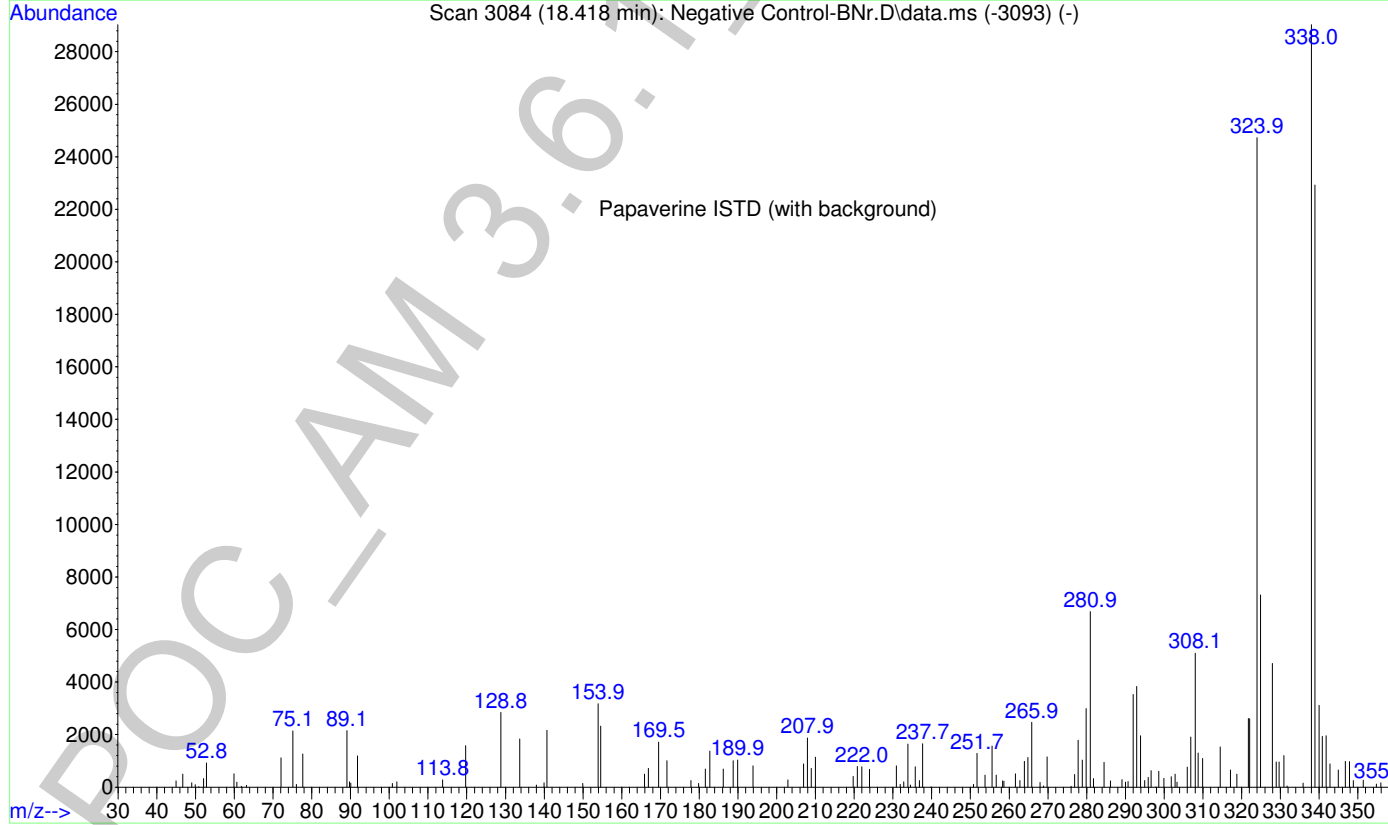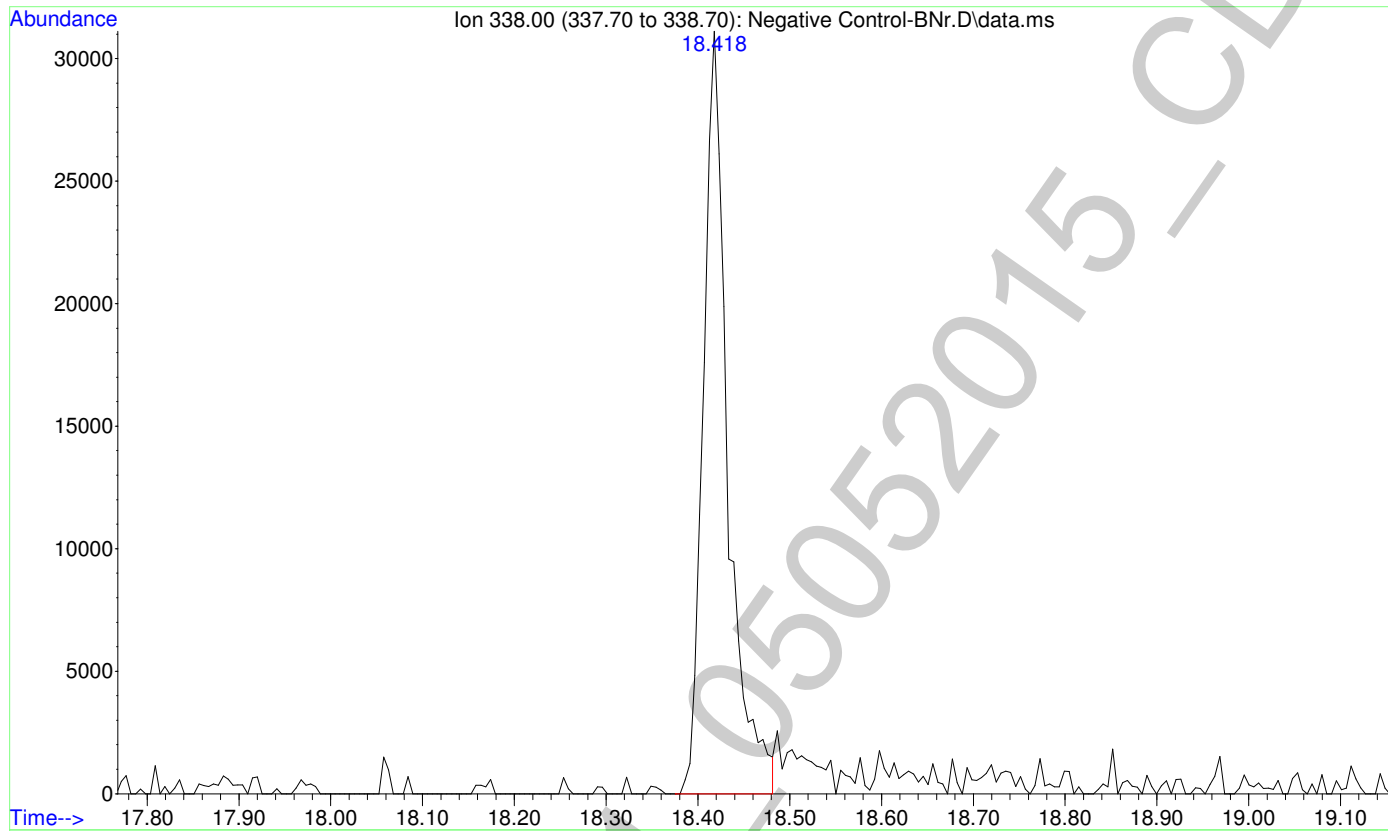



6

File :F:\Data\050515\Spiked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 20:33 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

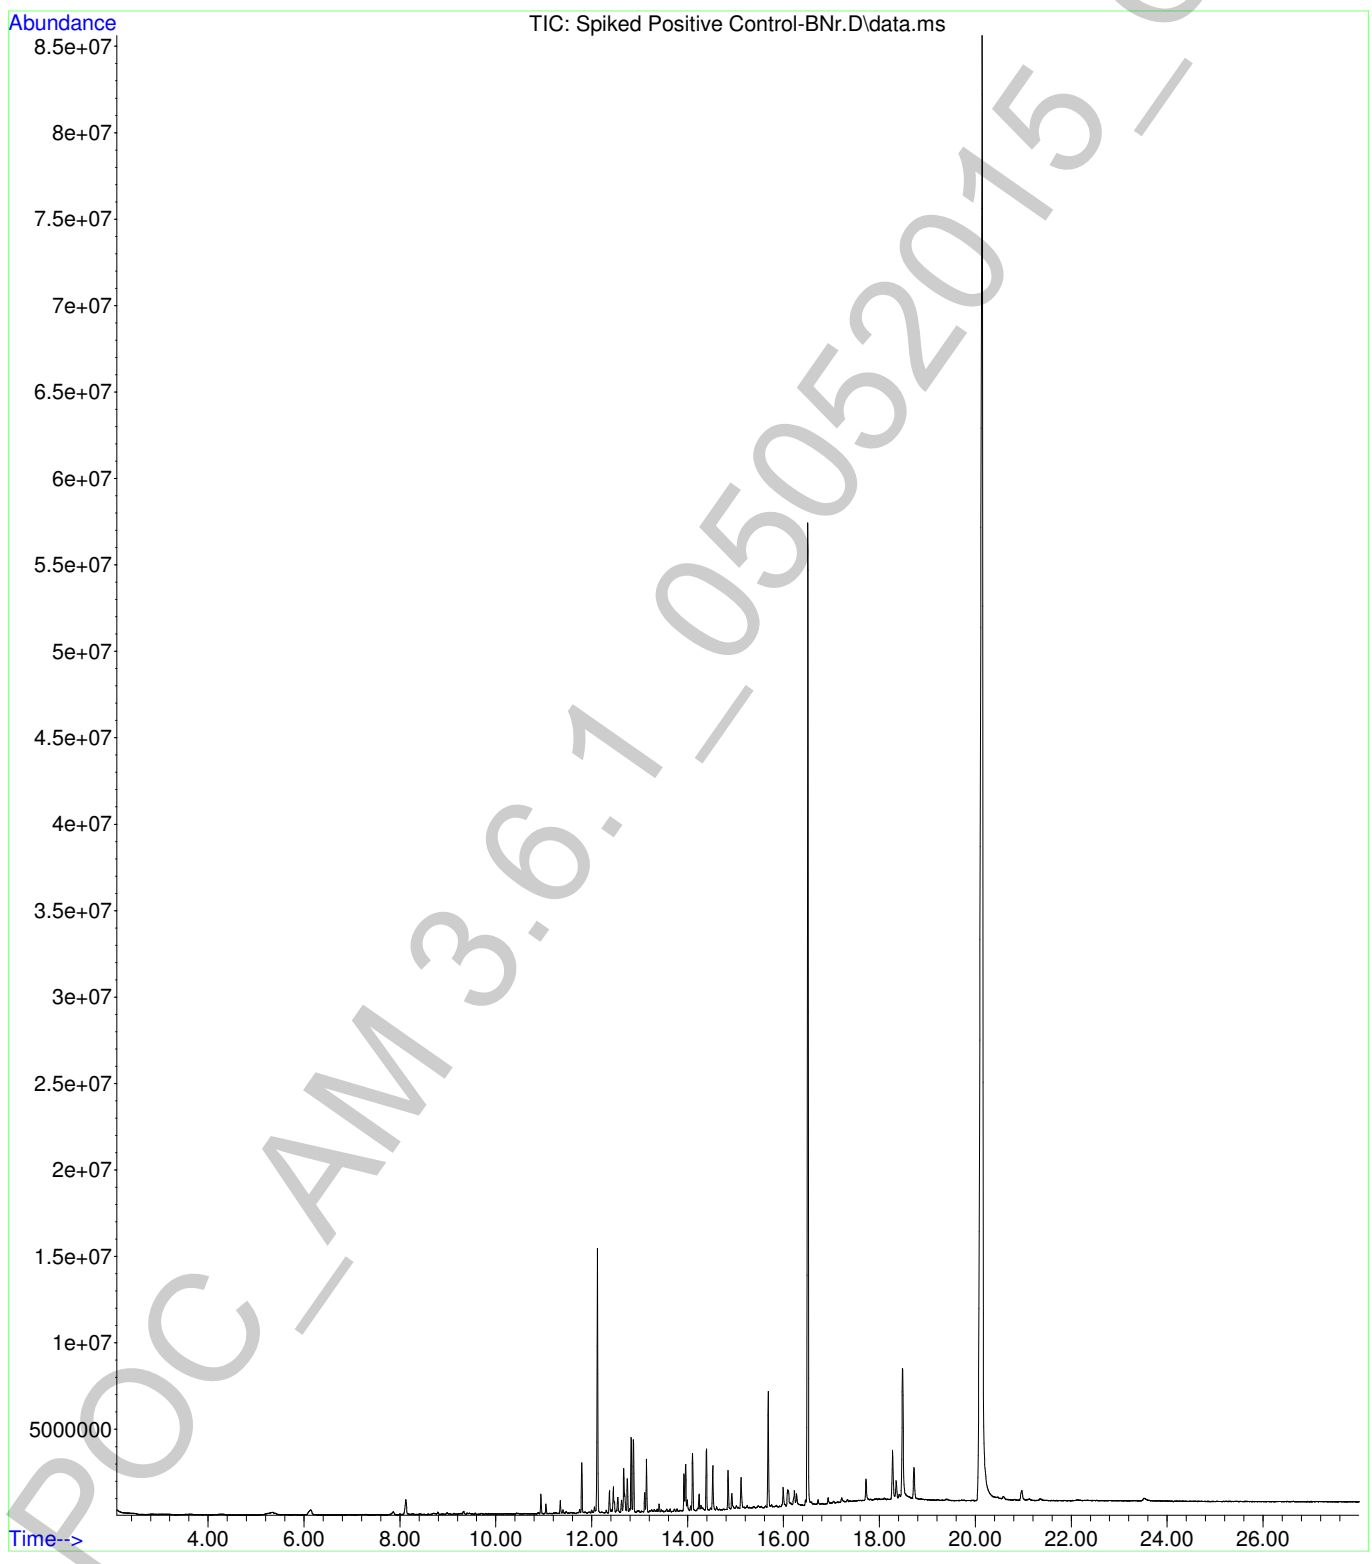



File :F:\Data\050515\Spiked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 20:33 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

2

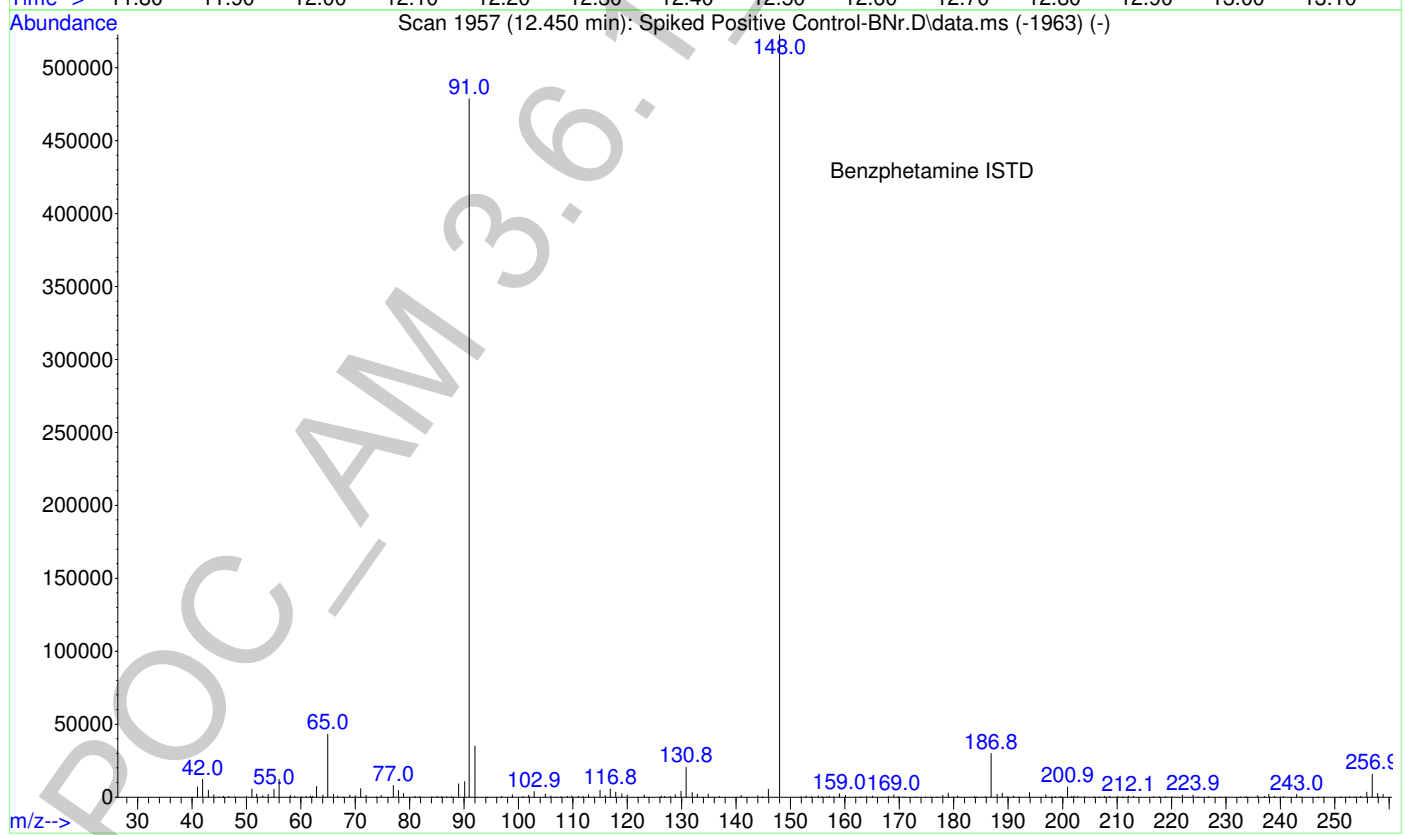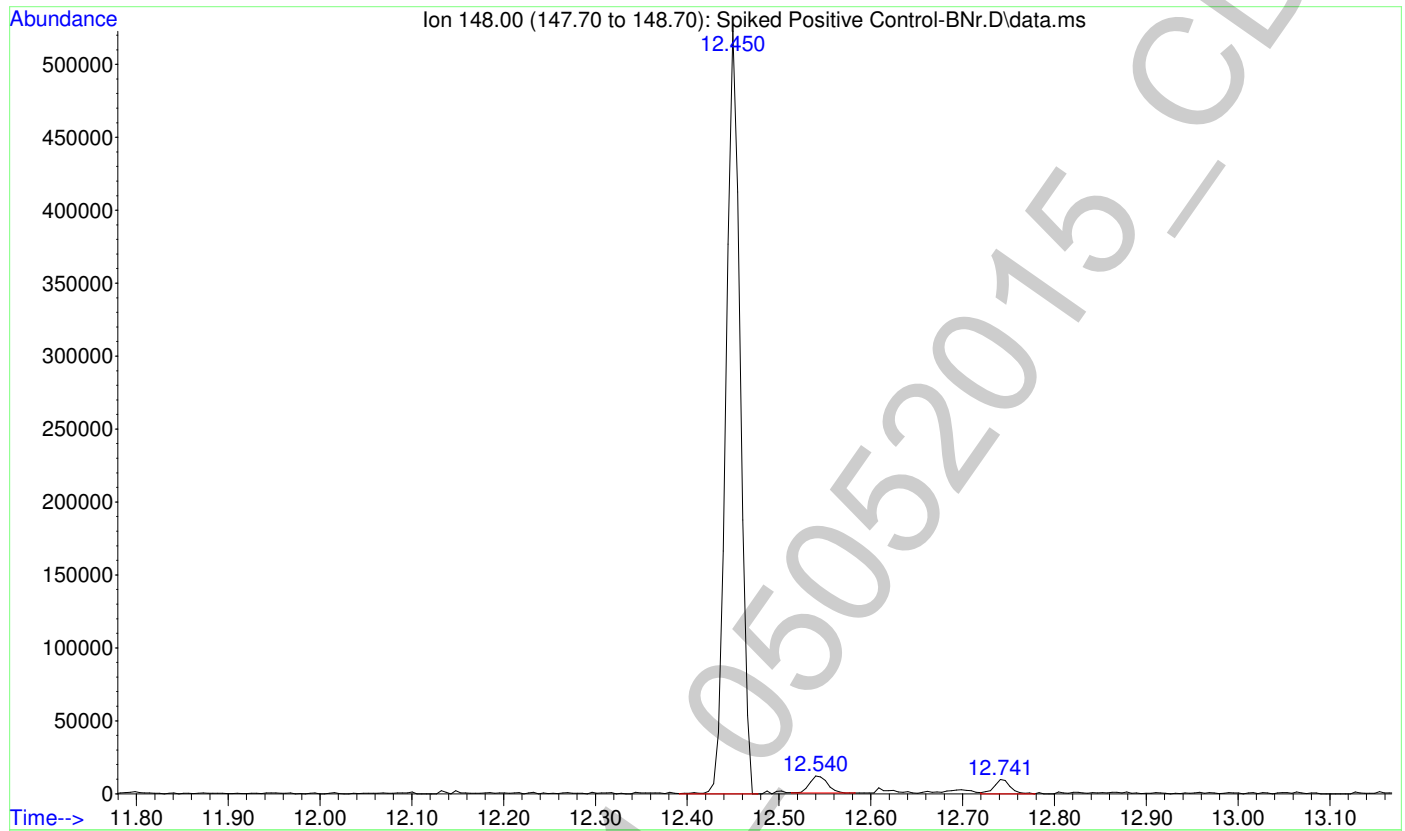



6

File :F:\Data\050515\Spiked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 20:33 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

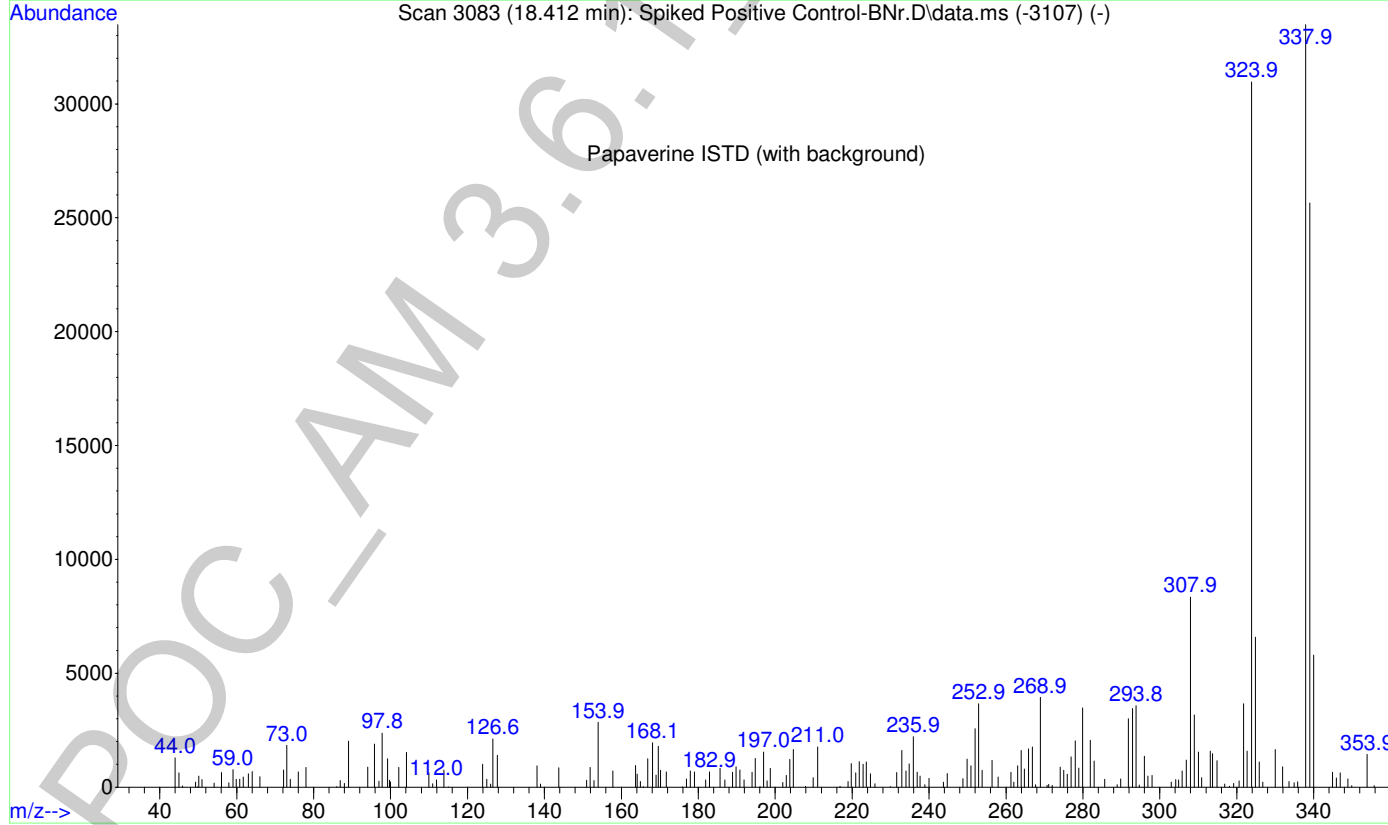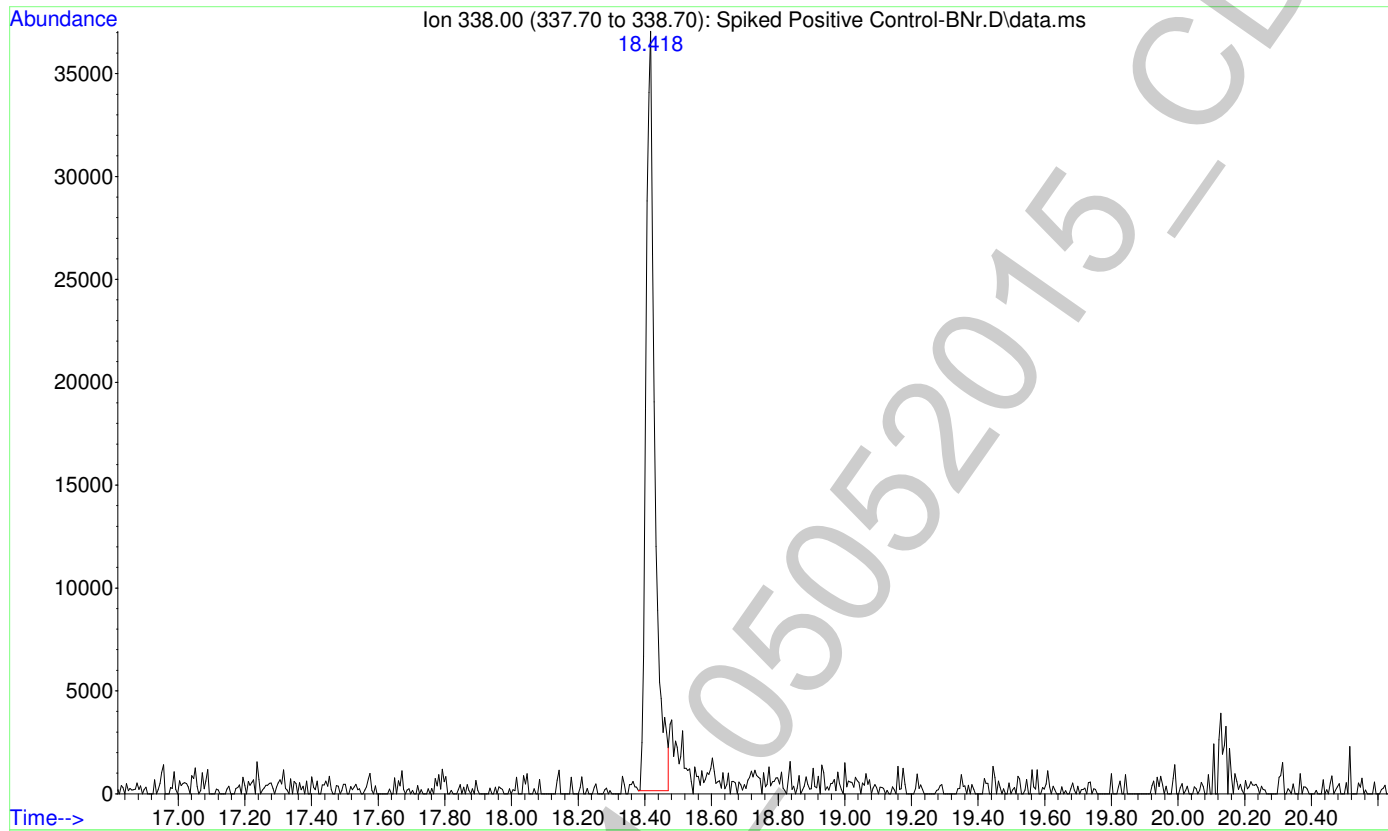



File :F:\Data\050515\Spiked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 20:33 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

6

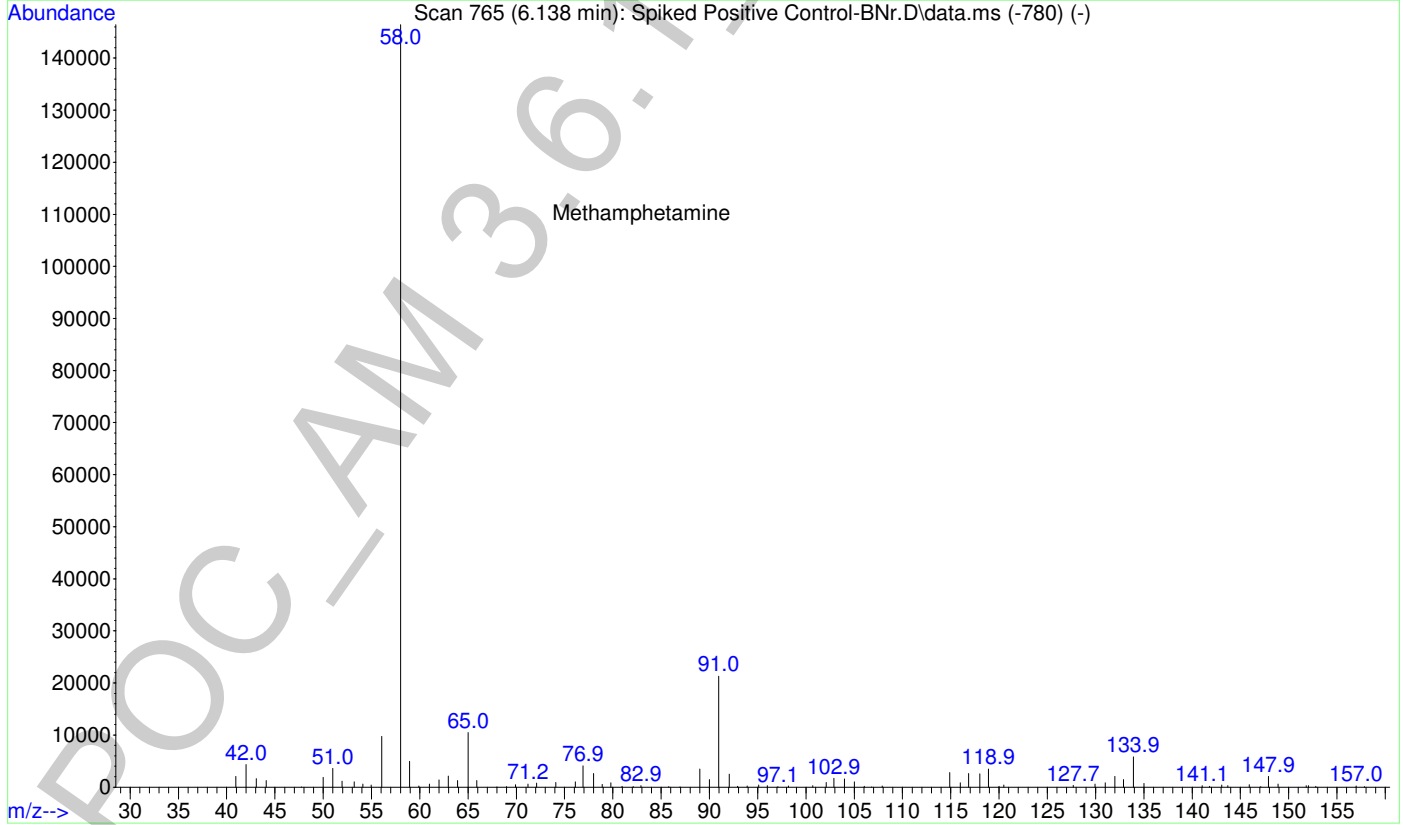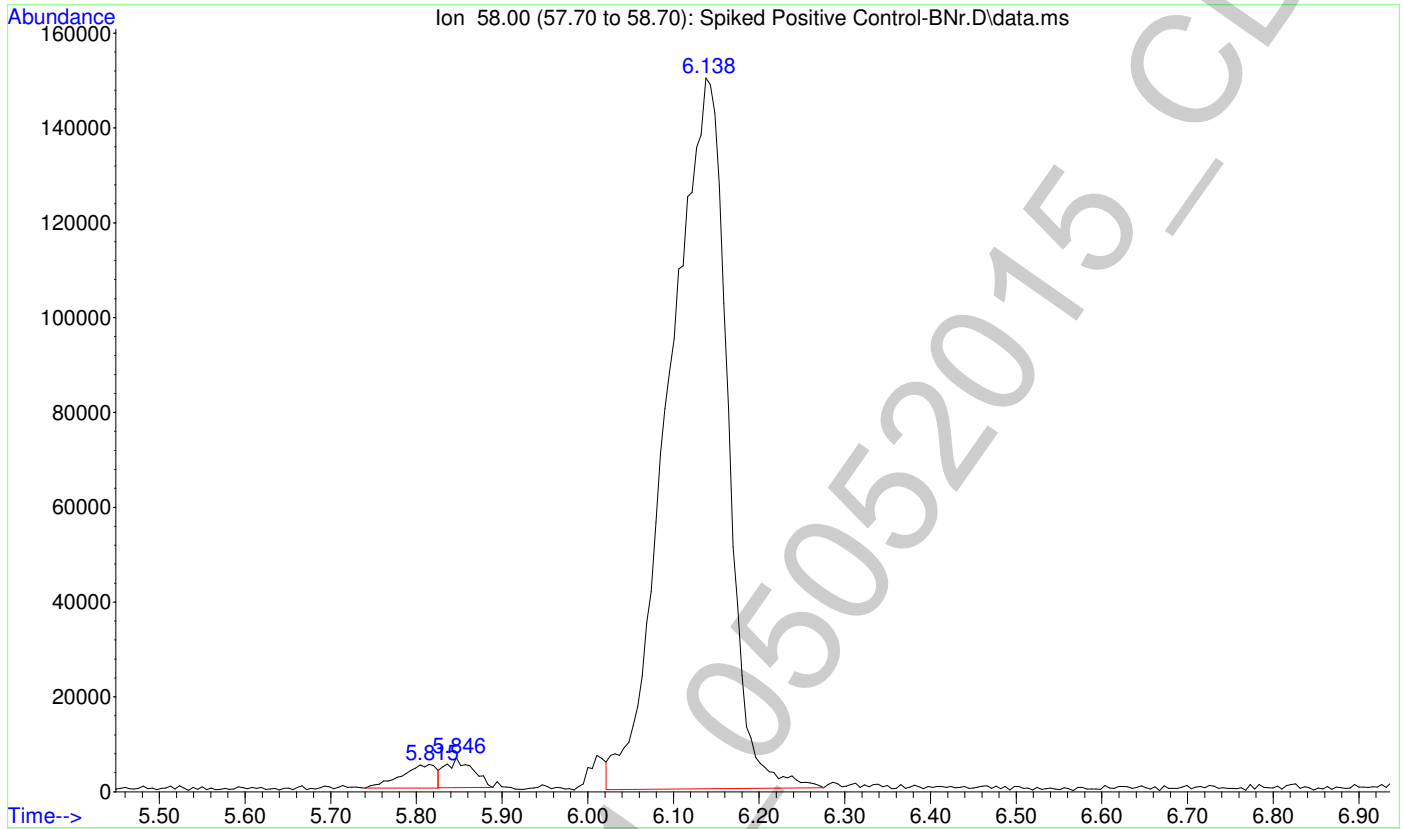



2

File :F:\Data\050515\Spiked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 20:33 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

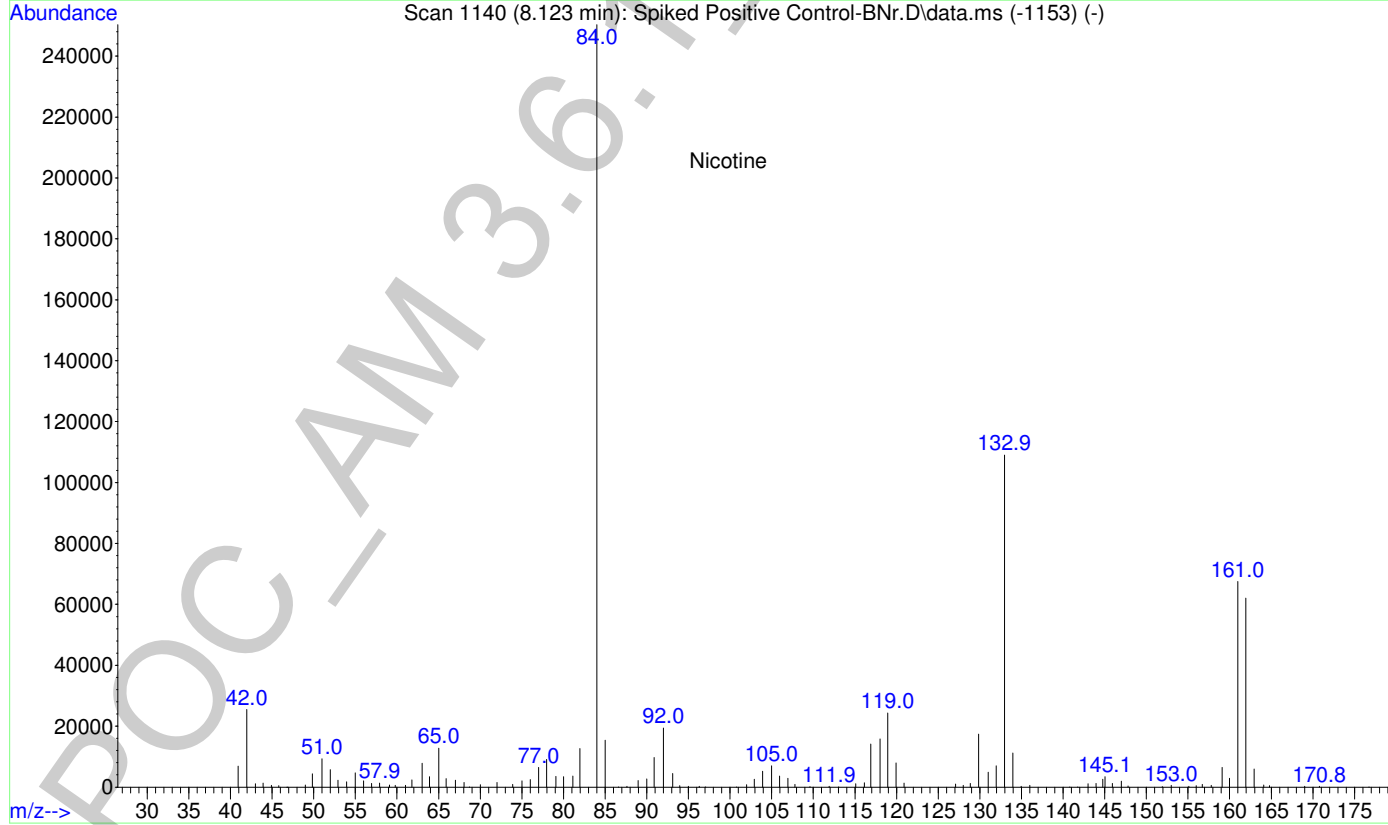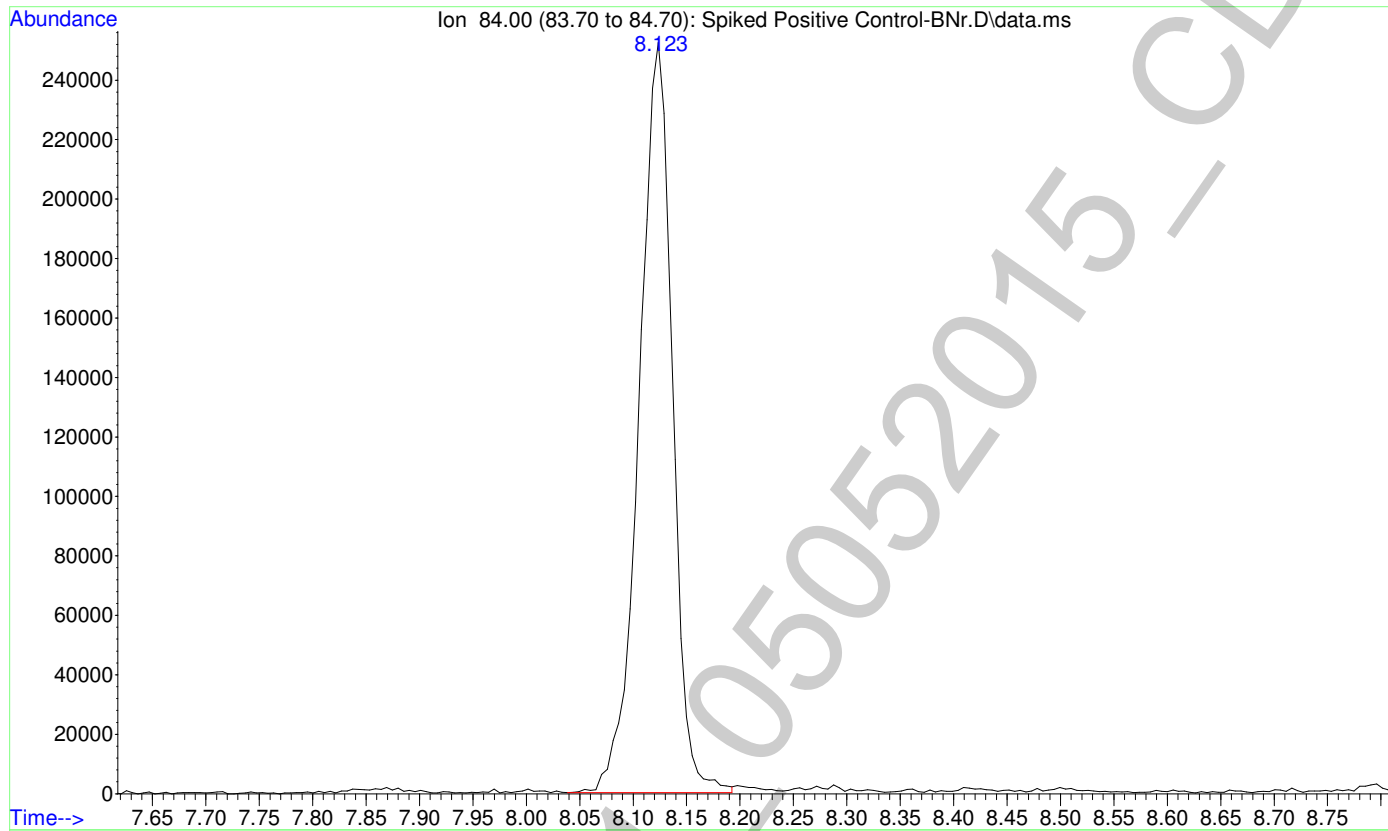



2

File :F:\Data\050515\Spiked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 20:33 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

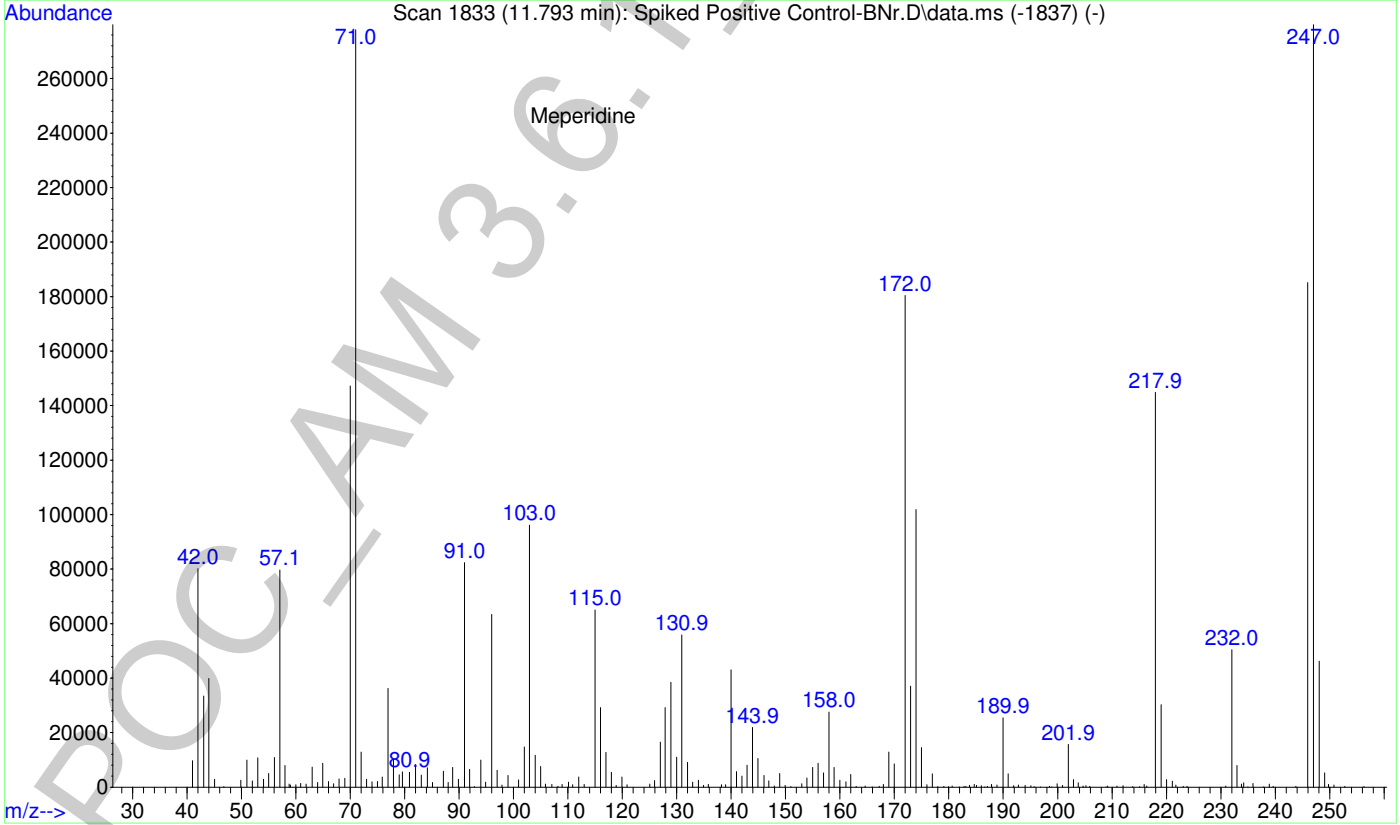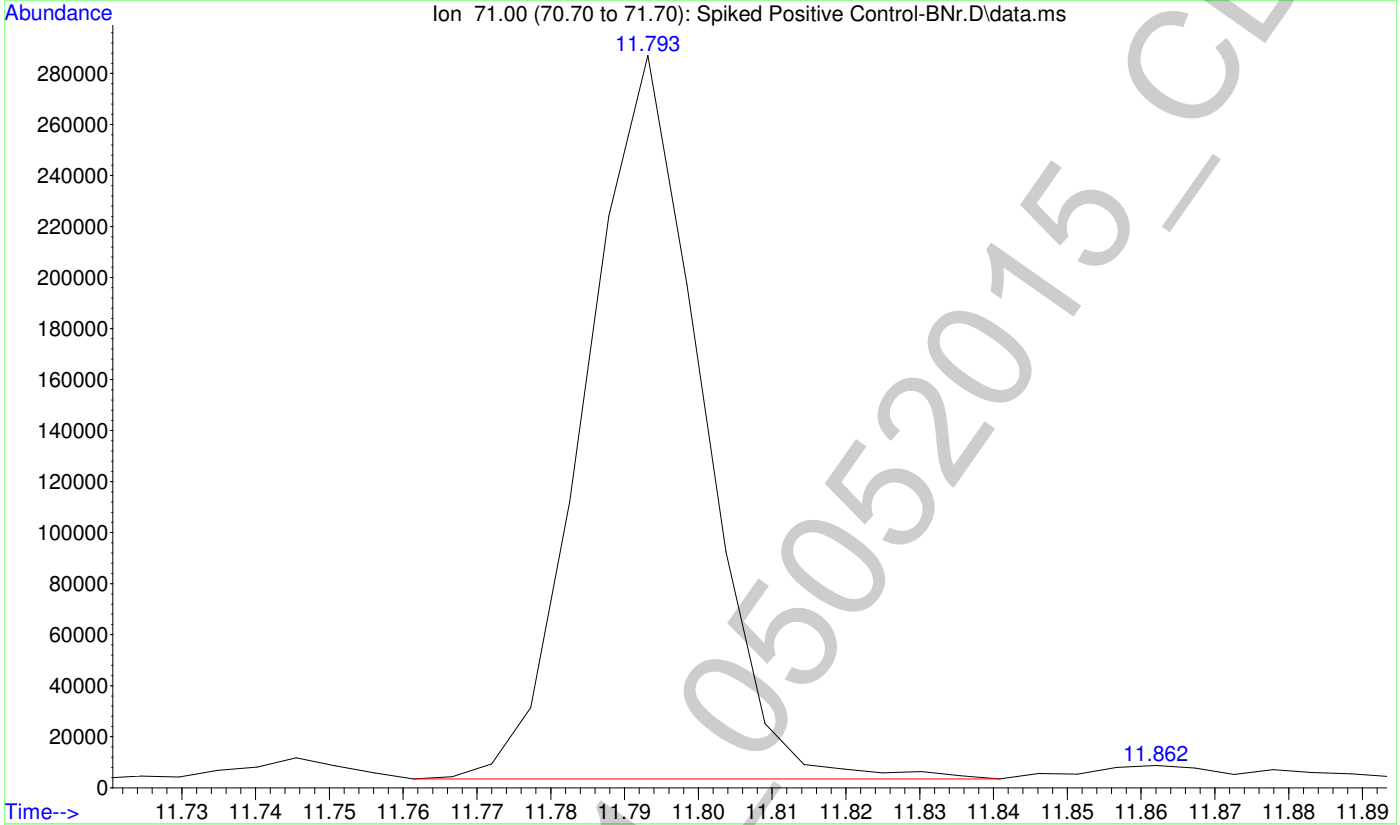



2

File :F:\Data\050515\Spiked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 20:33 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

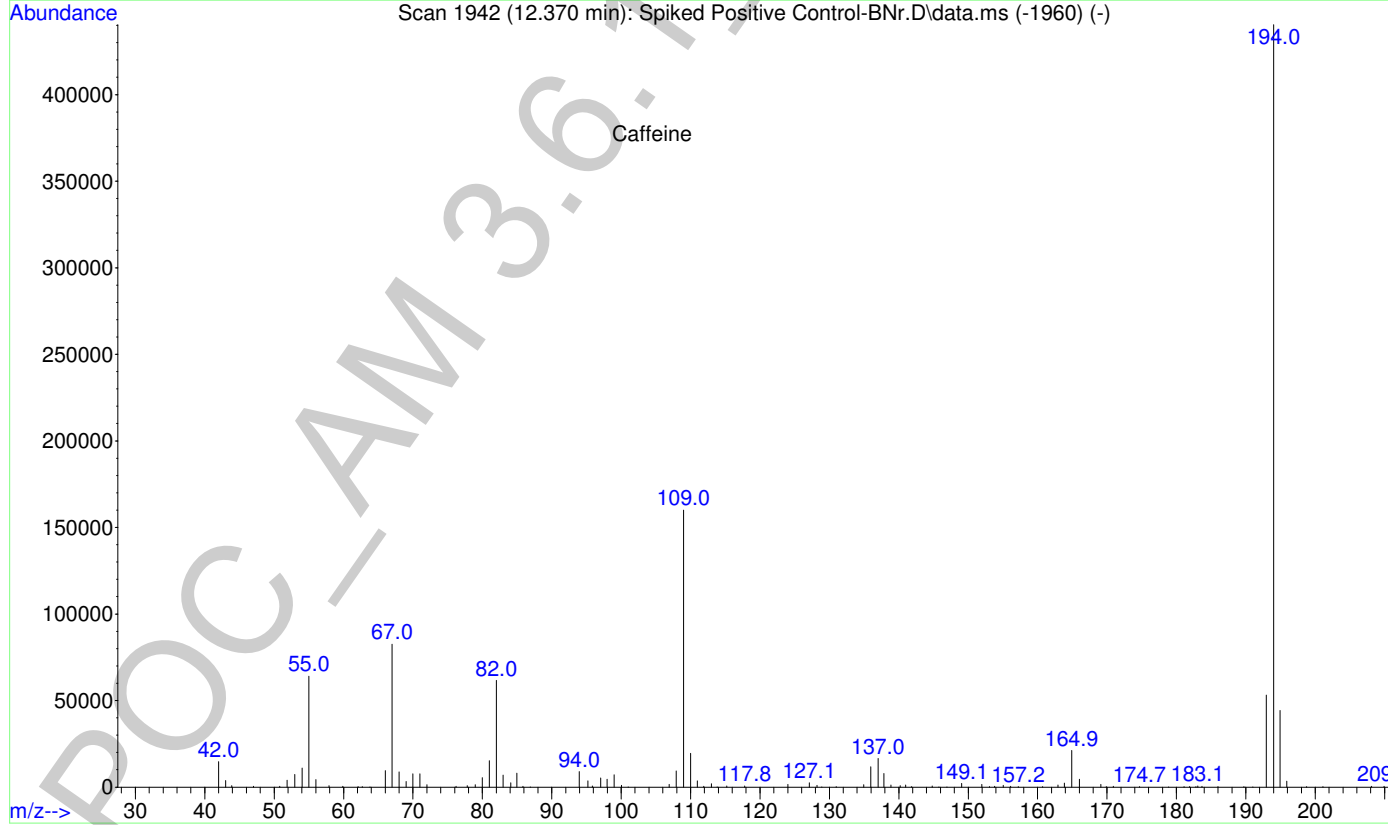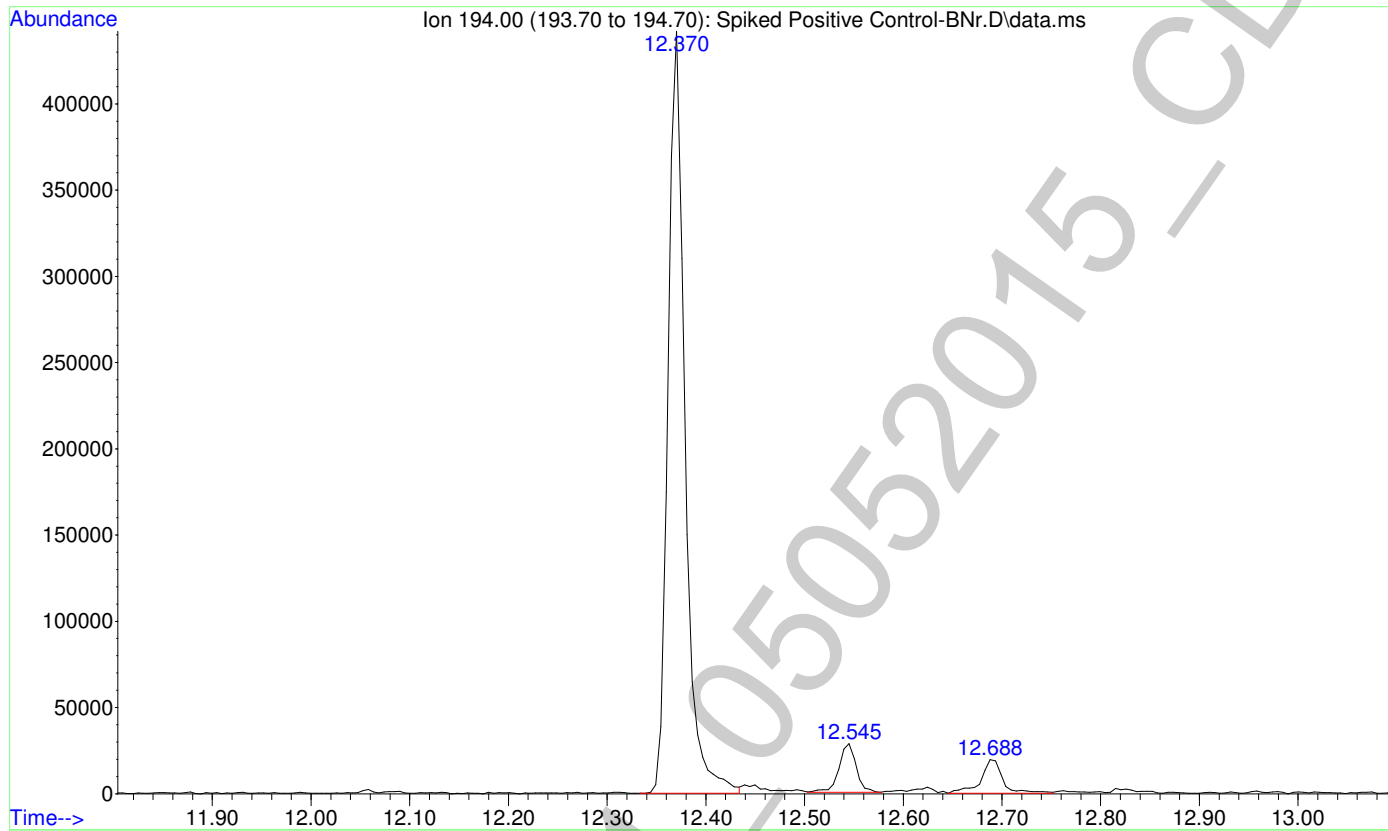



2

File :F:\Data\050515\Spiked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 20:33 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

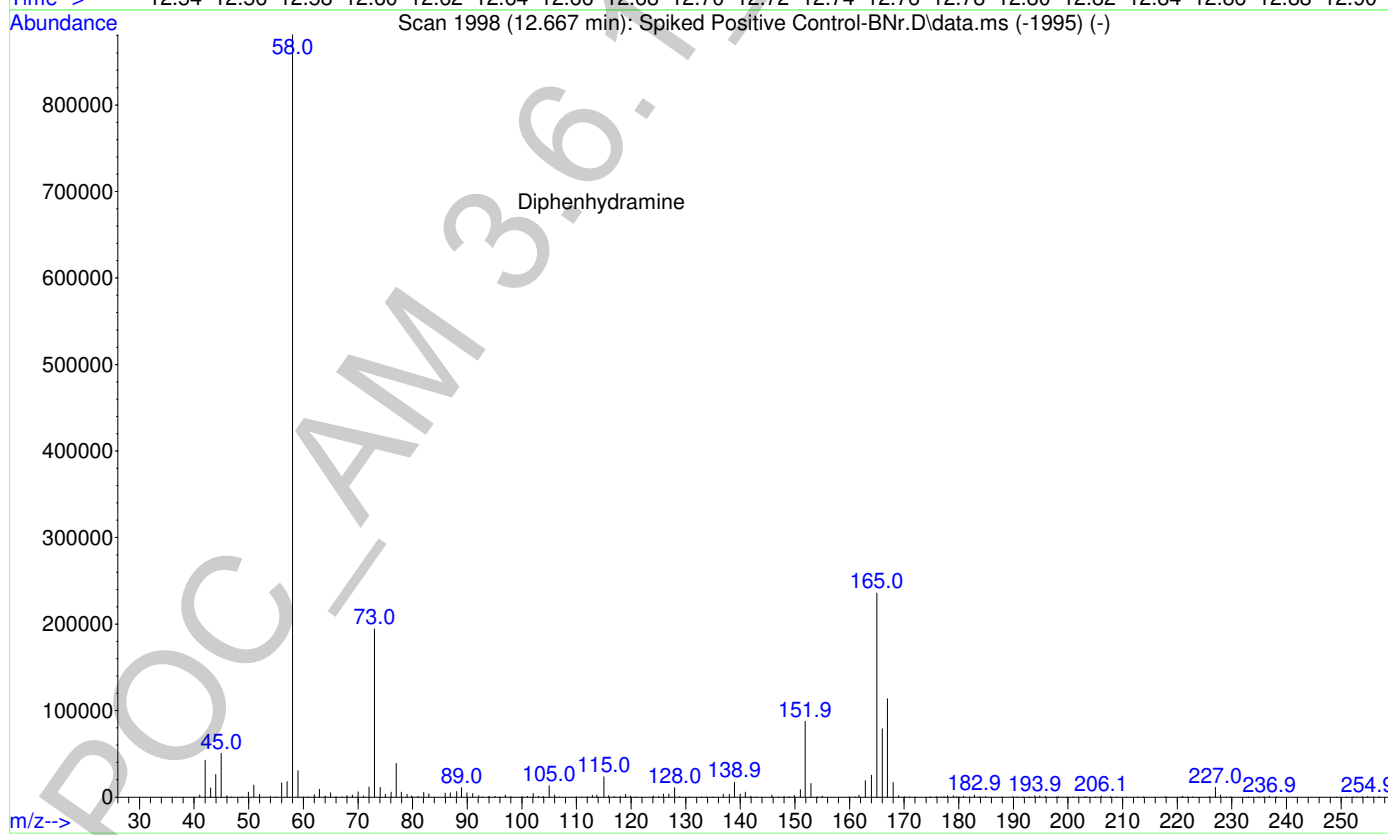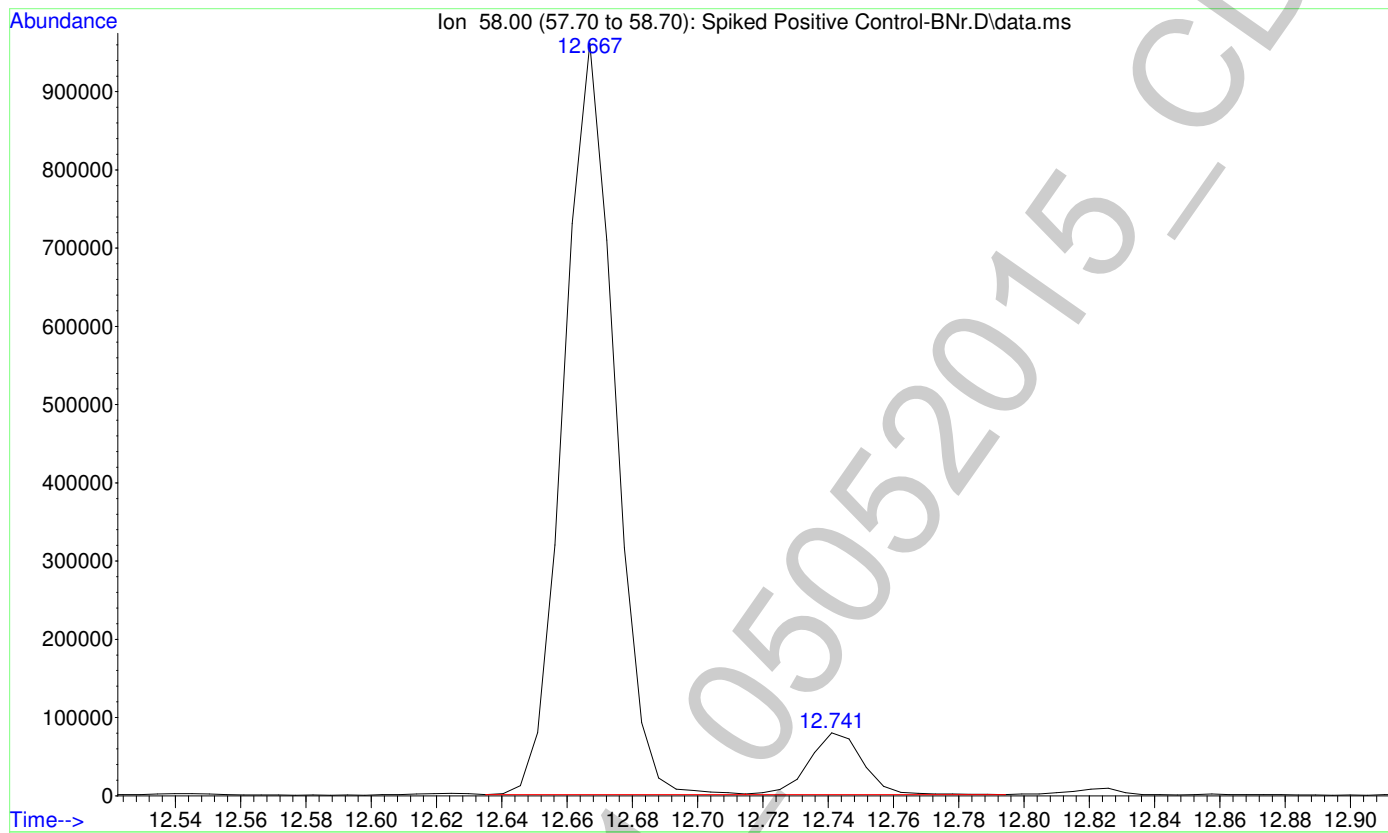



2

File :F:\Data\050515\Spiked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 20:33 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

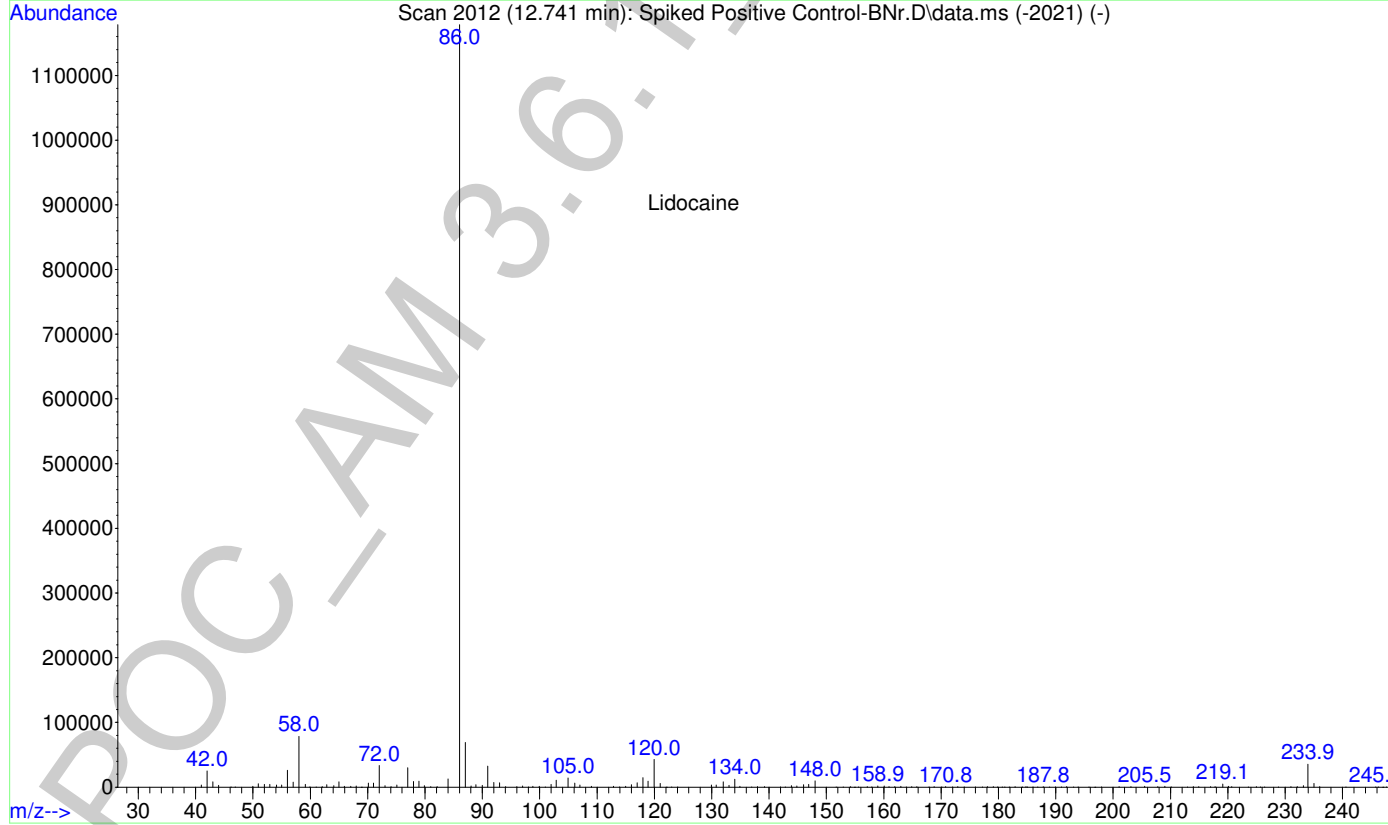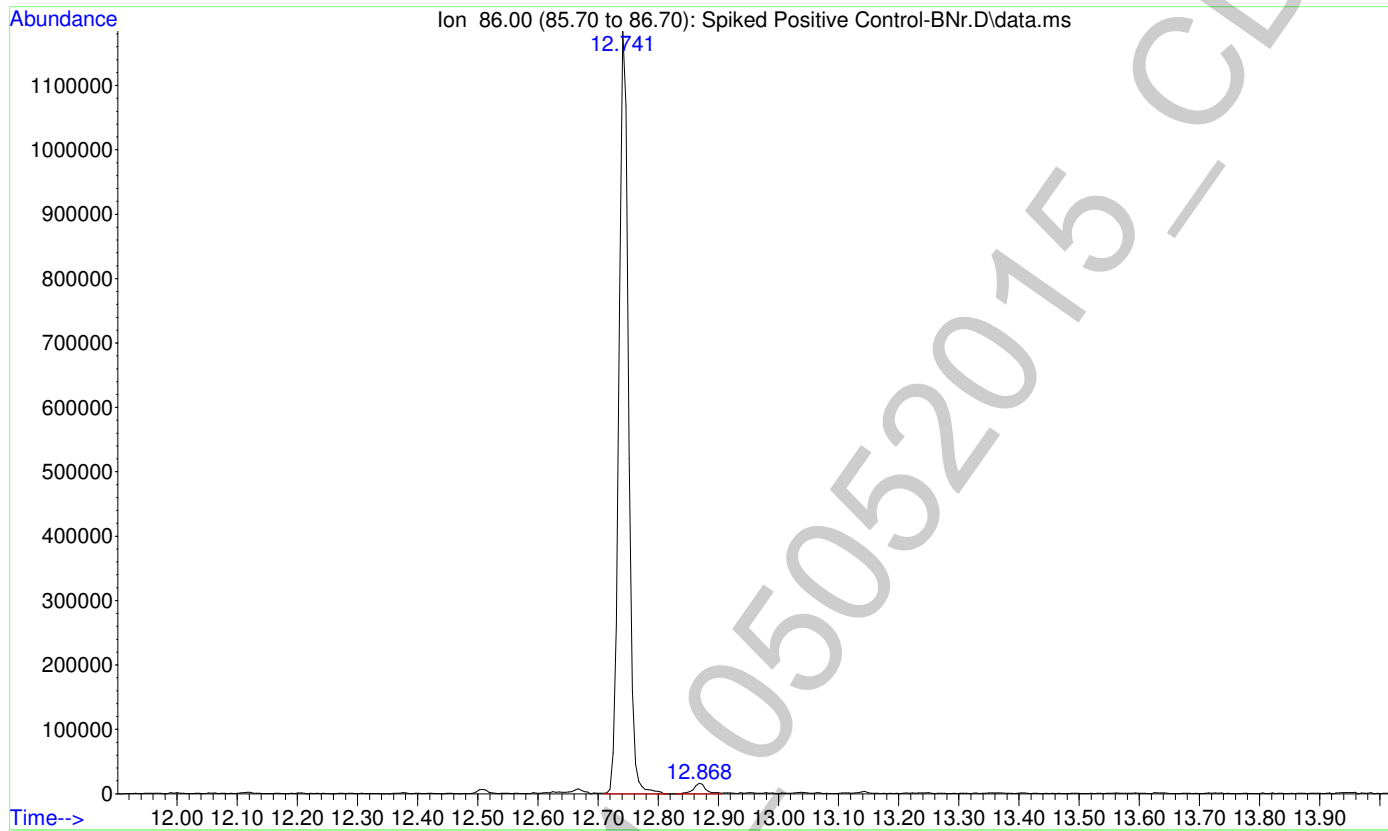



File : F:\Data\050515\Spiked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 20:33 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

2

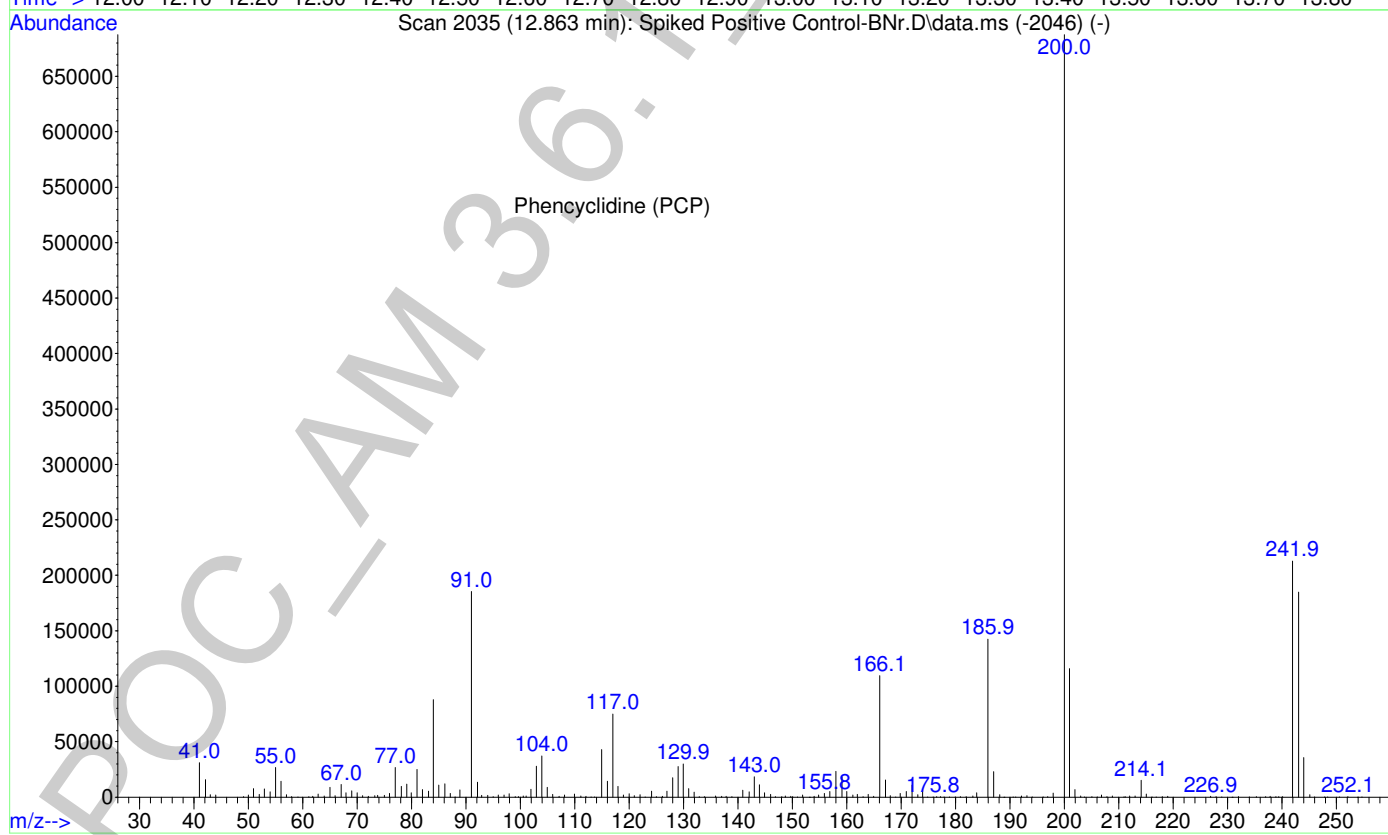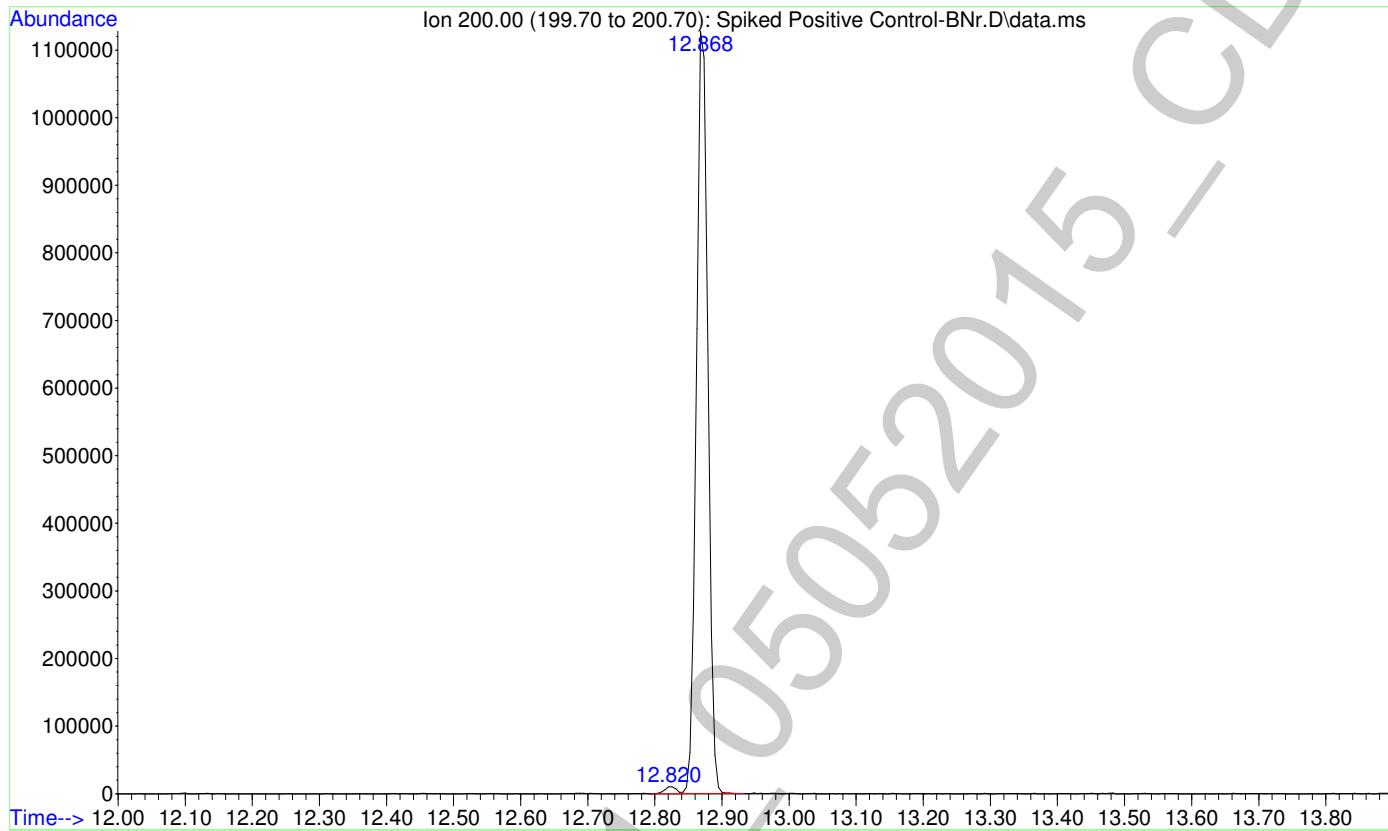



File :F:\Data\050515\Spiked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 20:33 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

2

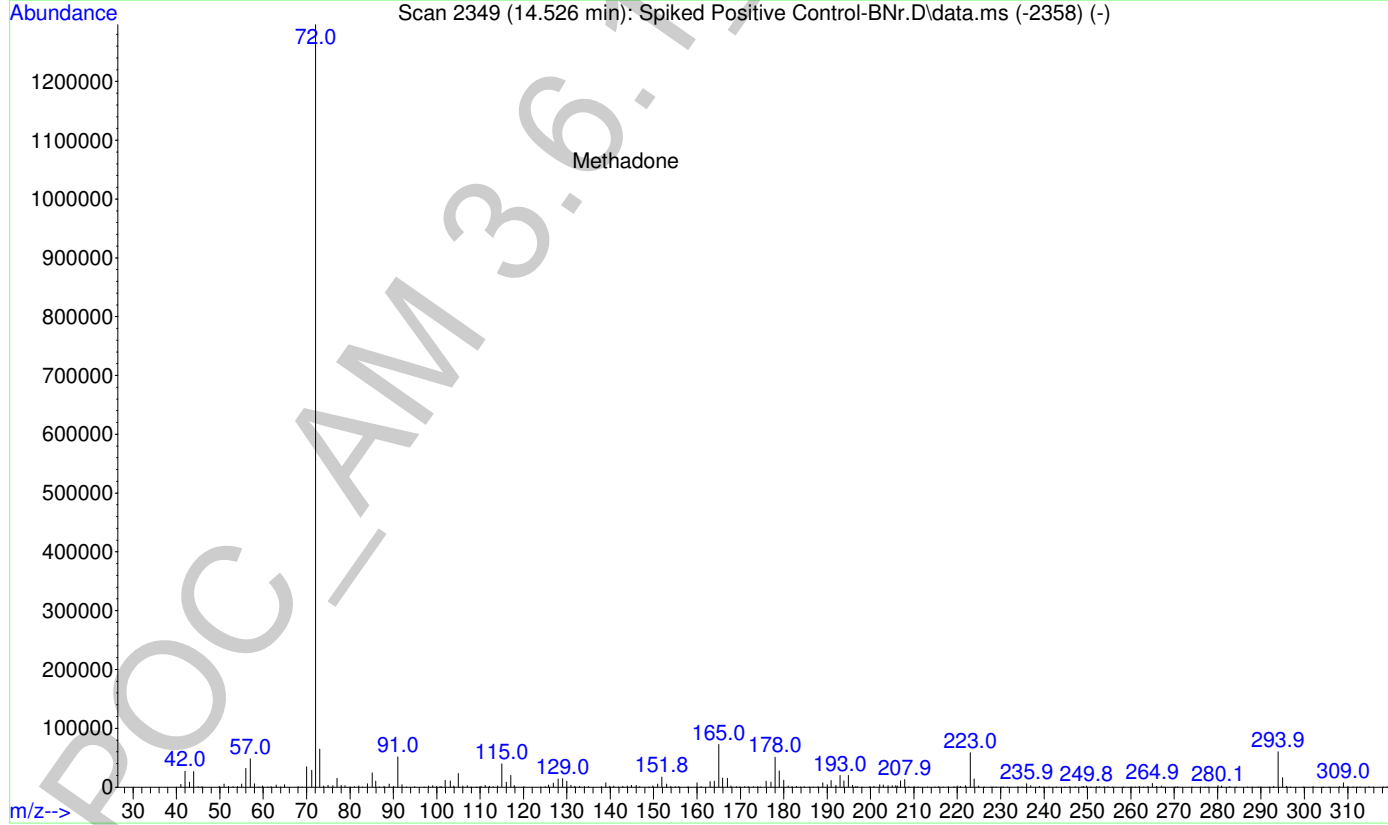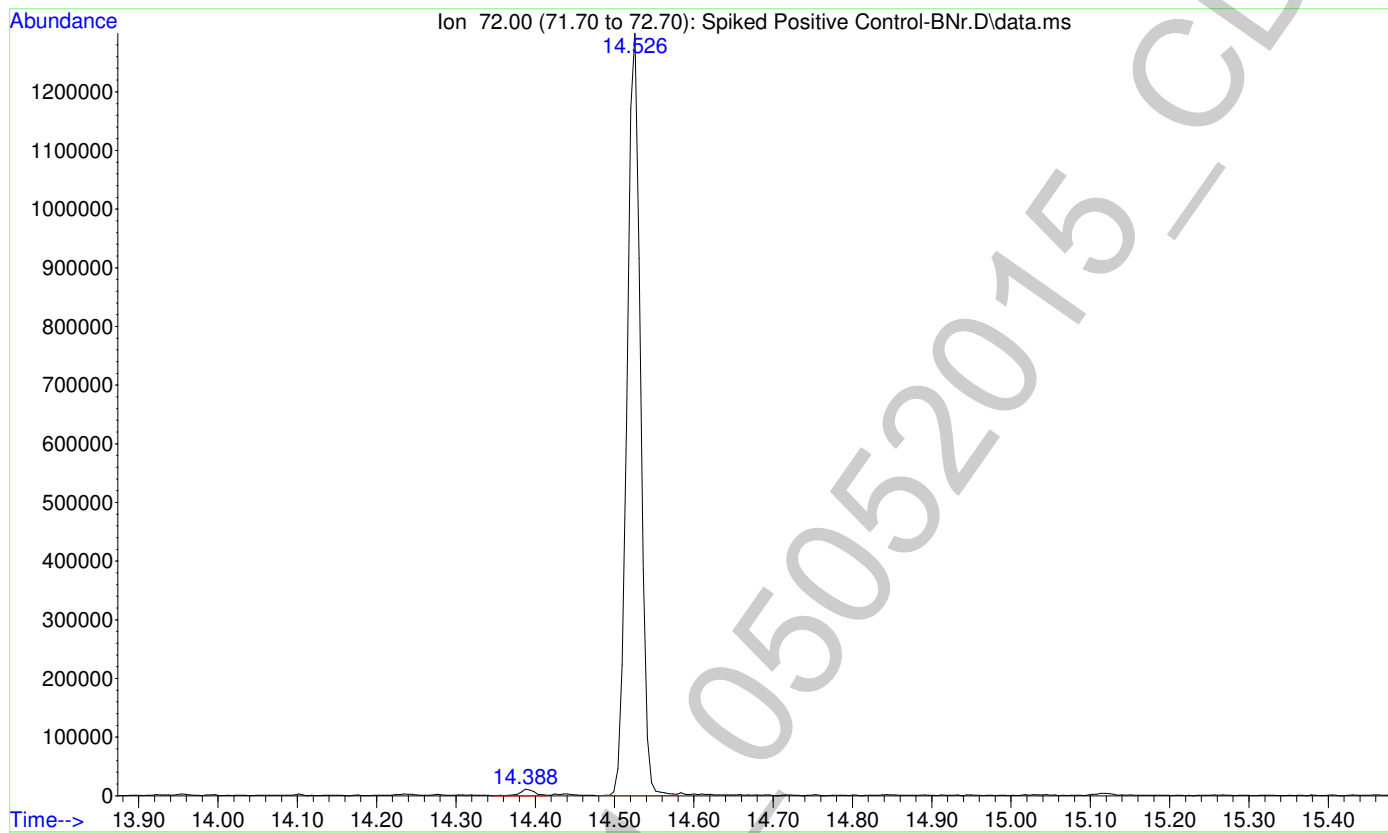



2

File :F:\Data\050515\Spiked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 20:33 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

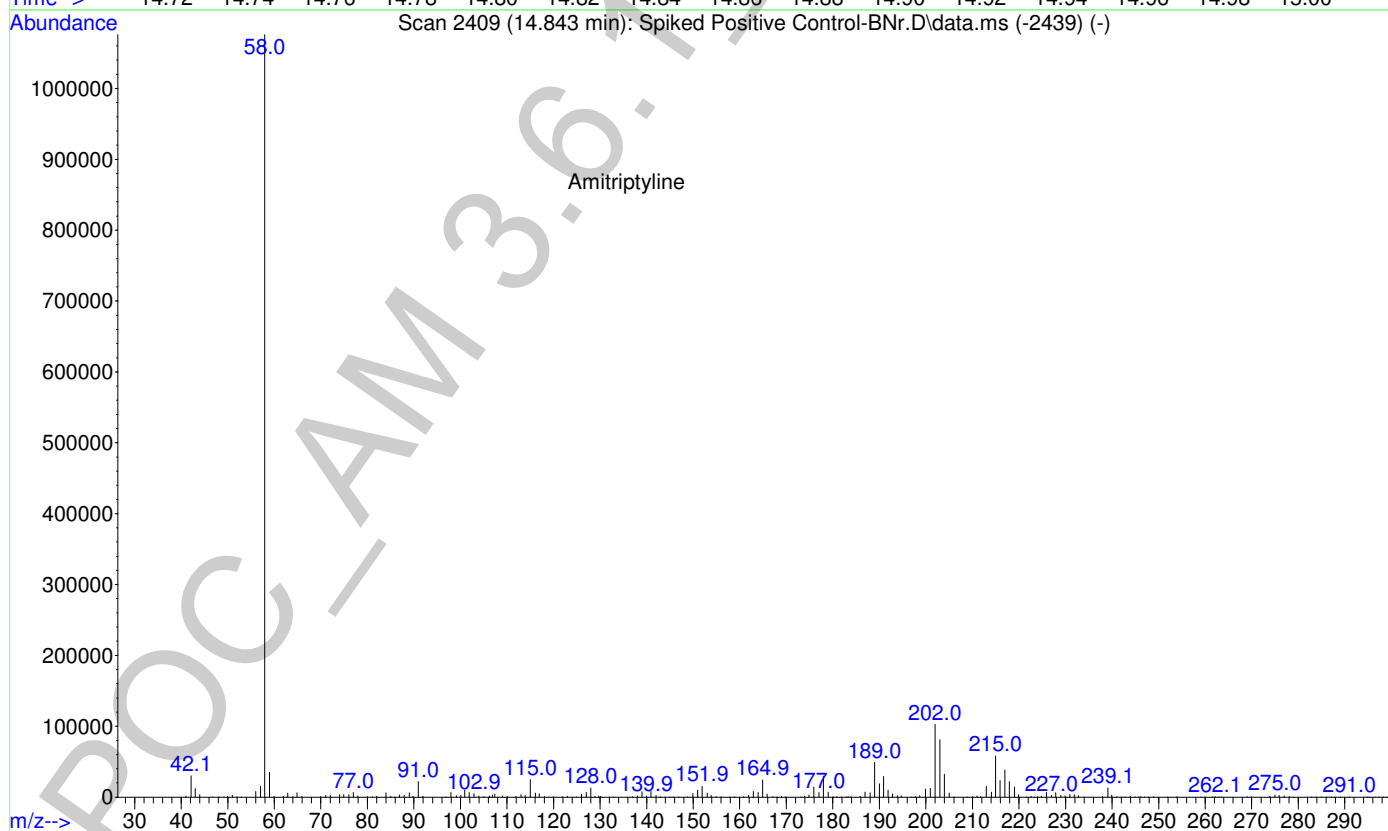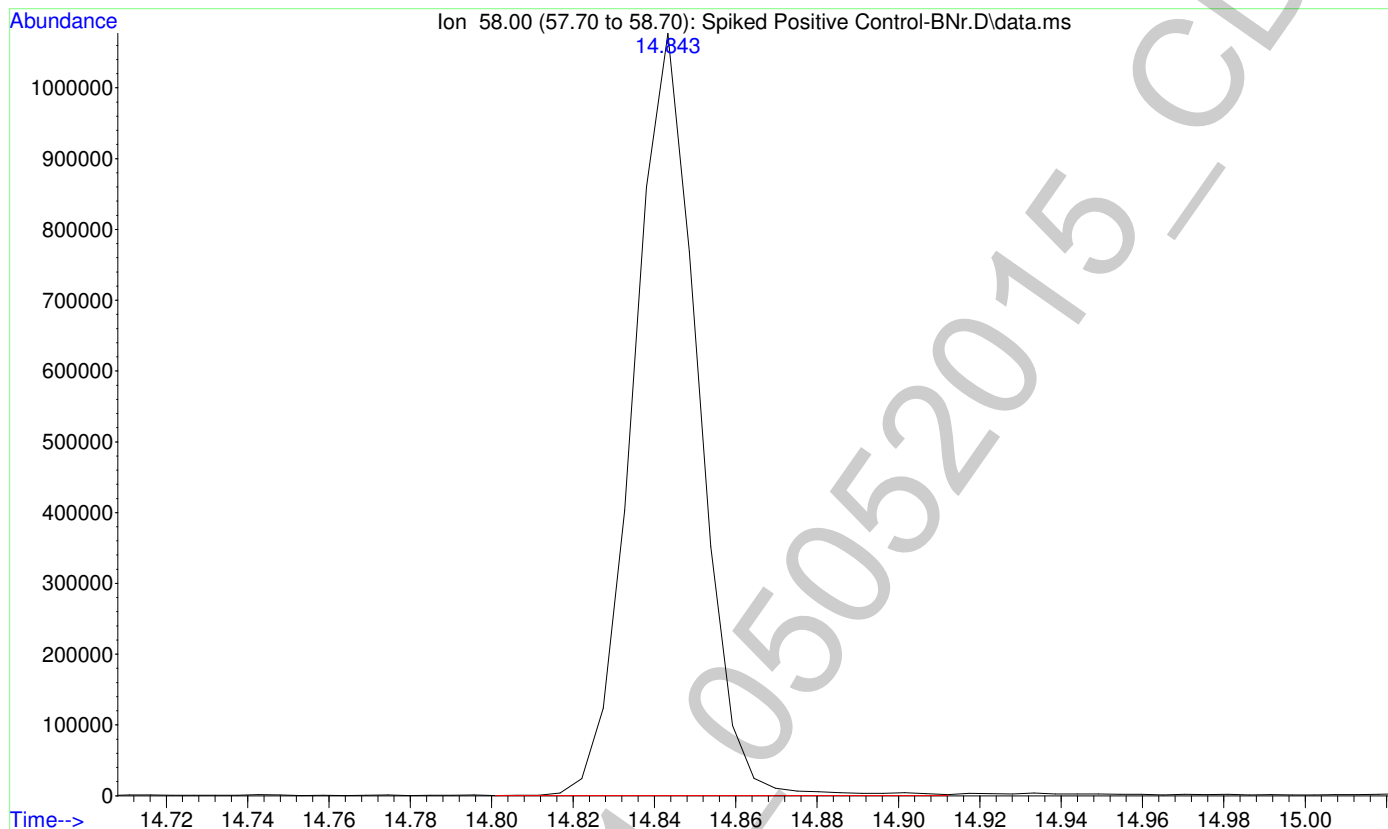

File :F:\Data\050515\Spiked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 20:33 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

2

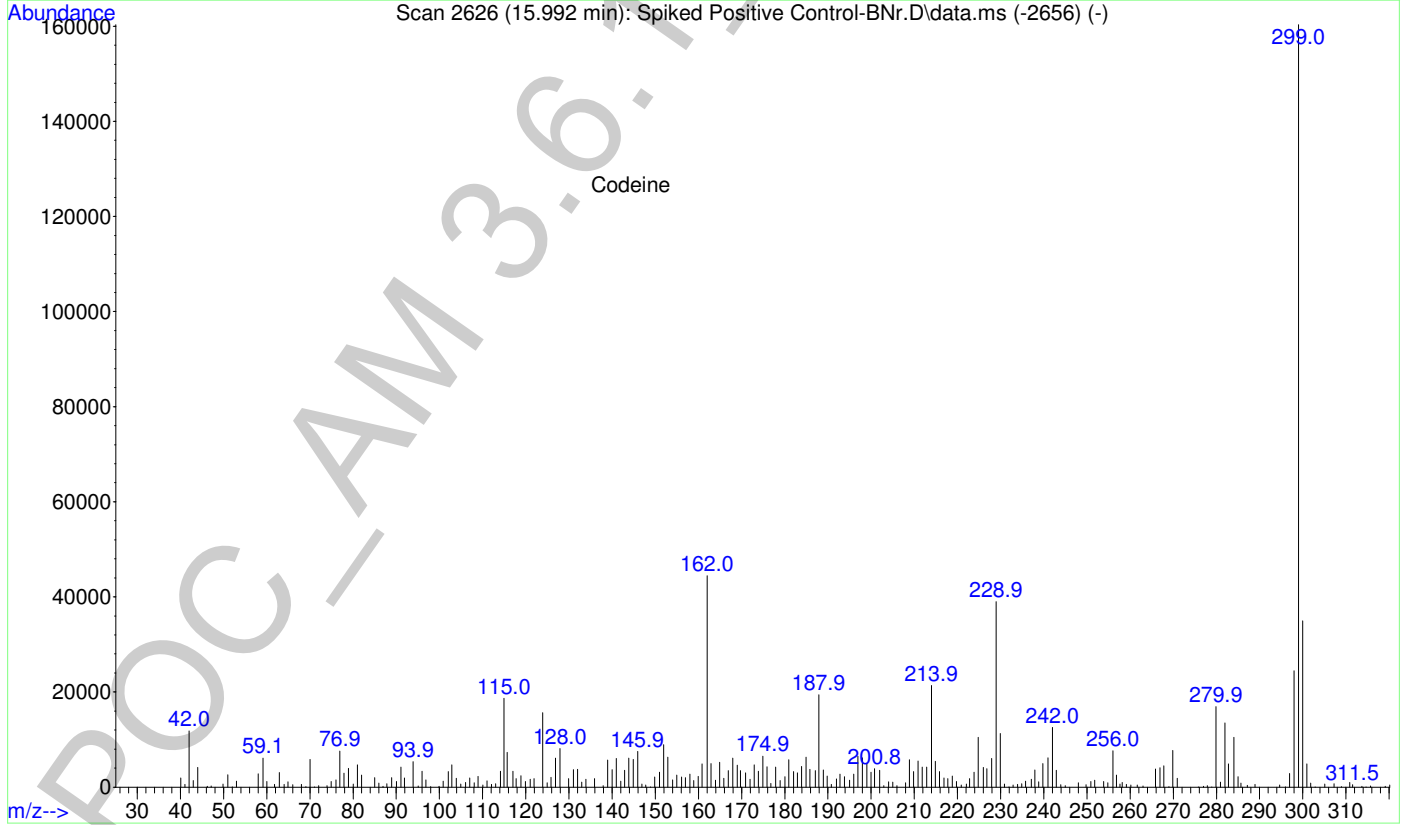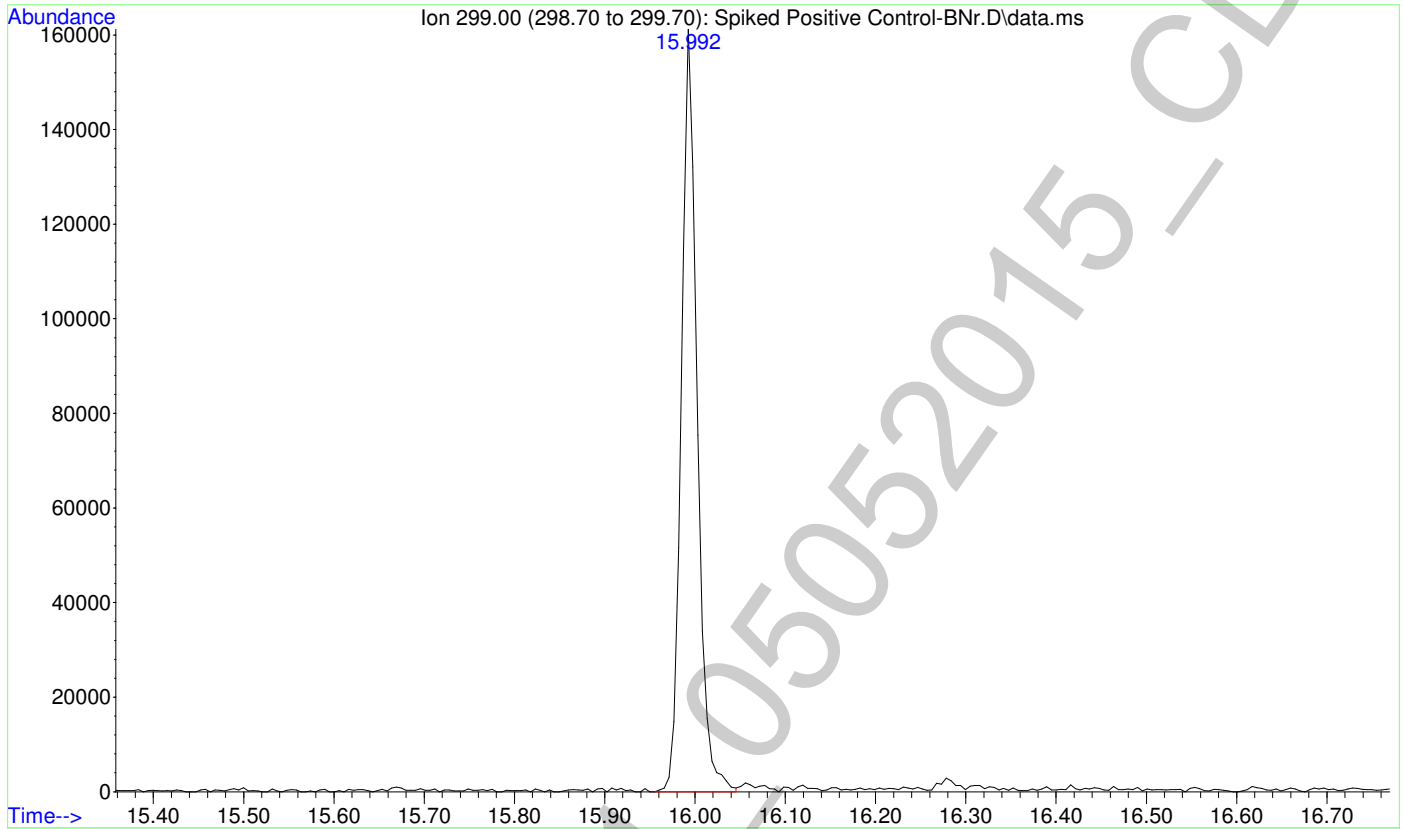

2

File :F:\Data\050515\Spiked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Acquired : 05 May 2015 20:33 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

