



7/22/2015

Worklist: 781


<u>LAB CASE</u>	<u>ITEM</u>	<u>TASK ID</u>	<u>DESCRIPTION</u>	
C2015-0862	1	33895	3.6.1 Blood base neutral confirr	
C2015-0892	1	34160	3.6.1 Blood base neutral confirr	
C2015-0920	1	34333	3.6.1 Blood base neutral confirr	
C2015-0931	1	34694	3.6.1 Blood base neutral confirr	
C2015-1016	1	35514	3.6.1 Blood base neutral confirr	
C2015-1039	1	35722	3.6.1 Blood base neutral confirr	
C2015-1041	1	35753	3.6.1 Blood base neutral confirr	
C2015-1074	2	36085	3.6.1 Blood base neutral confirr	
C2015-1079	1	36102	3.6.1 Blood base neutral confirr	
C2015-1098	1	36258	3.6.1 Blood base neutral confirr	
C2015-1182	1	36927	3.6.1 Blood base neutral confirr	
M2015-1819	1	38089	3.6.1 Blood base neutral confirr	
M2015-2063	1	36069	3.6.1 Blood base neutral confirr	
M2015-2088	1	36146	3.6.1 Blood base neutral confirr	
M2015-2121	1	36236	3.6.1 Blood base neutral confirr	
M2015-2146	1	36312	3.6.1 Blood base neutral confirr	
M2015-2152	1	36326	3.6.1 Blood base neutral confirr	
M2015-2160	1	36394	3.6.1 Blood base neutral confirr	
M2015-2161	1	37601	3.6.1 Blood base neutral confirr	
M2015-2161	2	37594	3.6.1 Blood base neutral confirr	
M2015-2162	1	36399	3.6.1 Blood base neutral confirr	
M2015-2178	1	36460	3.6.1 Blood base neutral confirr	
M2015-2179	1	36465	3.6.1 Blood base neutral confirr	

POC-AM36102



Worklist: 781

<u>LAB_CASE</u>	<u>ITEM</u>	<u>TASK_ID</u>	<u>DESCRIPTION</u>
M2015-2192	1	36503	3.6.1 Blood base neutral confirr
M2015-2194	1	36542	3.6.1 Blood base neutral confirr
M2015-2243	1	36767	3.6.1 Blood base neutral confirr
M2015-2243	2	37950	3.6.1 Blood base neutral confirr
M2015-2417	2	37614	3.6.1 Blood base neutral confirr
P2015-1534	1	36696	3.6.1 Blood base neutral confirr

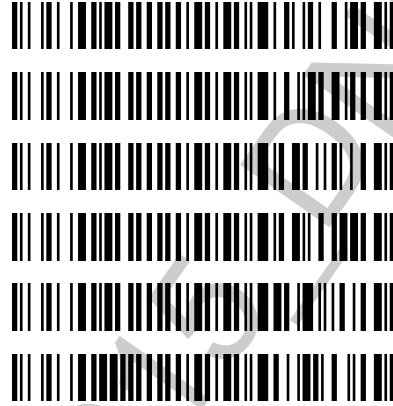


Reviewed: By Anne Nord 8/4/15

Reviewed on 8/5/15 by CS

POC_AM 3.6.1_072420



Verified ALS vials in correct positions in instrument rack on 07/24/2015. 

simulate_sequence.log
Simulate Run Sequence Fri Jul 24 11:13:42 2015


Instrument Name: Major Mass Spec
Sequence File: C:\Users\ISPuser\Desktop\Sequences\DD-BNSB072415.sequence.xml
Comment: MassHunter sequence
Operator: ISP\datastor
Data Path: D:\DATA\DND\2015\072415\
Method Path: D:\MassHunter\GCMS\1\methods\


Line	Type	Vials	DataFile	Sample Name
Acquisition Method: BNSB120510.M				
1)	Sample	100	Prerun Solvent Blank	Pre-run Solvent Blank
2)	Sample	1	Negative Control-BN	Negative Control -
...0689				
3)	Sample	2	Spiked Positive Control-BN	Positive Control
4)	Sample	99	prBLK2	Solvent Blank
Acquisition Method: GBT092509-Delta EMV.M				
5)	Sample	100	Prerun Solvent Blankr	Pre-run Solvent Blank
6)	Sample	1	Negative Control-BNr	Negative Control -
...0689				
7)	Sample	2	Spiked Positive Control-BNr	Positive Control
8)	Sample	99	prBLK2r	Solvent Blank
Acquisition Method: BNSB120510.M				
9)	Sample	98	C2015-0862-1-BNBLK	Lab No.: C2015-0862-1
10)	Sample	3	C2015-0862-1-BN	Lab No.: C2015-0862-1
11)	Sample	97	C2015-0892-1-BNBLK	Lab No.: C2015-0892-1
12)	Sample	4	C2015-0892-1-BN	Lab No.: C2015-0892-1
13)	Sample	96	C2015-0920-1-BNBLK	Lab No.: C2015-0920-1
14)	Sample	5	C2015-0920-1-BN	Lab No.: C2015-0920-1
15)	Sample	95	C2015-0931-1-BNBLK	Lab No.: C2015-0931-1
16)	Sample	6	C2015-0931-1-BN	Lab No.: C2015-0931-1
17)	Sample	94	C2015-1016-1-BNBLK	Lab No.: C2015-1016-1
18)	Sample	7	C2015-1016-1-BN	Lab No.: C2015-1016-1
19)	Sample	93	C2015-1039-1-BNBLK	Lab No.: C2015-1039-1
20)	Sample	8	C2015-1039-1-BN	Lab No.: C2015-1039-1
21)	Sample	92	C2015-1041-1-BNBLK	Lab No.: C2015-1041-1
22)	Sample	9	C2015-1041-1-BN	Lab No.: C2015-1041-1
23)	Sample	91	C2015-1074-2-BNBLK	Lab No.: C2015-1074-2
24)	Sample	10	C2015-1074-2-BN	Lab No.: C2015-1074-2
Acquisition Method: GBT092509-Delta EMV.M				
25)	Sample	98	C2015-0862-1-BNBLKr	Lab No.: C2015-0862-1
26)	Sample	3	C2015-0862-1-BNr	Lab No.: C2015-0862-1
27)	Sample	97	C2015-0892-1-BNBLKr	Lab No.: C2015-0892-1
28)	Sample	4	C2015-0892-1-BNr	Lab No.: C2015-0892-1
29)	Sample	96	C2015-0920-1-BNBLKr	Lab No.: C2015-0920-1
30)	Sample	5	C2015-0920-1-BNr	Lab No.: C2015-0920-1
31)	Sample	95	C2015-0931-1-BNBLKr	Lab No.: C2015-0931-1
32)	Sample	6	C2015-0931-1-BNr	Lab No.: C2015-0931-1
33)	Sample	94	C2015-1016-1-BNBLKr	Lab No.: C2015-1016-1
34)	Sample	7	C2015-1016-1-BNr	Lab No.: C2015-1016-1
35)	Sample	93	C2015-1039-1-BNBLKr	Lab No.: C2015-1039-1
36)	Sample	8	C2015-1039-1-BNr	Lab No.: C2015-1039-1
37)	Sample	92	C2015-1041-1-BNBLKr	Lab No.: C2015-1041-1
38)	Sample	9	C2015-1041-1-BNr	Lab No.: C2015-1041-1
39)	Sample	91	C2015-1074-2-BNBLKr	Lab No.: C2015-1074-2
40)	Sample	10	C2015-1074-2-BNr	Lab No.: C2015-1074-2
Acquisition Method: BNSB120510.M				
41)	Sample	90	C2015-1079-1-BNBLK	Lab No.: C2015-1079-1
42)	Sample	11	C2015-1079-1-BN	Lab No.: C2015-1079-1
43)	Sample	89	C2015-1098-1-BNBLK	Lab No.: C2015-1098-1
44)	Sample	12	C2015-1098-1-BN	Lab No.: C2015-1098-1



Verified ALS vials in correct positions in instrument rack on 07/24/2015.

		simulate_sequence.log			
45) Sample	88	C2015-1182-1-BNBLK	Lab No.:	C2015-1182-1	
46) Sample	13	C2015-1182-1-BN	Lab No.:	C2015-1182-1	
47) Sample	87	M2015-1819-1-BNBLK	Lab No.:	M2015-1819-1	
48) Sample	14	M2015-1819-1-BN	Lab No.:	M2015-1819-1	
49) Sample	86	M2015-2063-1-BNBLK	Lab No.:	M2015-2063-1	
50) Sample	15	M2015-2063-1-BN	Lab No.:	M2015-2063-1	
Acquisition Method: GBT092509-Delta EMV.M					
51) Sample	90	C2015-1079-1-BNBLK	Lab No.:	C2015-1079-1	
52) Sample	11	C2015-1079-1-BNr	Lab No.:	C2015-1079-1	
53) Sample	89	C2015-1098-1-BNBLK	Lab No.:	C2015-1098-1	
54) Sample	12	C2015-1098-1-BNr	Lab No.:	C2015-1098-1	
55) Sample	88	C2015-1182-1-BNBLK	Lab No.:	C2015-1182-1	
56) Sample	13	C2015-1182-1-BNr	Lab No.:	C2015-1182-1	
57) Sample	87	M2015-1819-1-BNBLK	Lab No.:	M2015-1819-1	
58) Sample	14	M2015-1819-1-BNr	Lab No.:	M2015-1819-1	
59) Sample	86	M2015-2063-1-BNBLK	Lab No.:	M2015-2063-1	
60) Sample	15	M2015-2063-1-BNr	Lab No.:	M2015-2063-1	
Acquisition Method: BNSB120510.M					
61) Sample	85	M2015-2088-1-BNBLK	Lab No.:	M2015-2088-1	
62) Sample	16	M2015-2088-1-BN	Lab No.:	M2015-2088-1	
63) Sample	84	M2015-2121-1-BNBLK	Lab No.:	M2015-2121-1	
64) Sample	17	M2015-2121-1-BN	Lab No.:	M2015-2121-1	
65) Sample	83	M2015-2146-1-BNBLK	Lab No.:	M2015-2146-1	
66) Sample	18	M2015-2146-1-BN	Lab No.:	M2015-2146-1	
67) Sample	82	M2015-2152-1-BNBLK	Lab No.:	M2015-2152-1	
68) Sample	19	M2015-2152-1-BN	Lab No.:	M2015-2152-1	
69) Sample	81	M2015-2160-1-BNBLK	Lab No.:	M2015-2160-1	
70) Sample	20	M2015-2160-1-BN	Lab No.:	M2015-2160-1	
Acquisition Method: GBT092509-Delta EMV.M					
71) Sample	85	M2015-2088-1-BNBLK	Lab No.:	M2015-2088-1	
72) Sample	16	M2015-2088-1-BNr	Lab No.:	M2015-2088-1	
73) Sample	84	M2015-2121-1-BNBLK	Lab No.:	M2015-2121-1	
74) Sample	17	M2015-2121-1-BNr	Lab No.:	M2015-2121-1	
75) Sample	83	M2015-2146-1-BNBLK	Lab No.:	M2015-2146-1	
76) Sample	18	M2015-2146-1-BNr	Lab No.:	M2015-2146-1	
77) Sample	82	M2015-2152-1-BNBLK	Lab No.:	M2015-2152-1	
78) Sample	19	M2015-2152-1-BNr	Lab No.:	M2015-2152-1	
79) Sample	81	M2015-2160-1-BNBLK	Lab No.:	M2015-2160-1	
80) Sample	20	M2015-2160-1-BNr	Lab No.:	M2015-2160-1	
Acquisition Method: BNSB120510.M					
81) Sample	80	M2015-2161-1-BNBLK	Lab No.:	M2015-2161-1	
82) Sample	21	M2015-2161-1-BN	Lab No.:	M2015-2161-1	
83) Sample	79	M2015-2161-2-BNBLK	Lab No.:	M2015-2161-2	
84) Sample	22	M2015-2161-2-BN	Lab No.:	M2015-2161-2	
85) Sample	78	M2015-2162-1-BNBLK	Lab No.:	M2015-2162-1	
86) Sample	23	M2015-2162-1-BN	Lab No.:	M2015-2162-1	
87) Sample	77	M2015-2178-1-BNBLK	Lab No.:	M2015-2178-1	
88) Sample	24	M2015-2178-1-BN	Lab No.:	M2015-2178-1	
89) Sample	76	M2015-2179-1B-BNBLK	Lab No.:	M2015-2179-1B	
90) Sample	25	M2015-2179-1B-BN	Lab No.:	M2015-2179-1B	
Acquisition Method: GBT092509-Delta EMV.M					
91) Sample	80	M2015-2161-1-BNBLK	Lab No.:	M2015-2161-1	
92) Sample	21	M2015-2161-1-BNr	Lab No.:	M2015-2161-1	
93) Sample	79	M2015-2161-2-BNBLK	Lab No.:	M2015-2161-2	
94) Sample	22	M2015-2161-2-BNr	Lab No.:	M2015-2161-2	
95) Sample	78	M2015-2162-1-BNBLK	Lab No.:	M2015-2162-1	
96) Sample	23	M2015-2162-1-BNr	Lab No.:	M2015-2162-1	
97) Sample	77	M2015-2178-1-BNBLK	Lab No.:	M2015-2178-1	
98) Sample	24	M2015-2178-1-BNr	Lab No.:	M2015-2178-1	
99) Sample	76	M2015-2179-1B-BNBLK	Lab No.:	M2015-2179-1B	
100) Sample	25	M2015-2179-1B-BNr	Lab No.:	M2015-2179-1B	
Acquisition Method: BNSB120510.M					



Verified ALS vials in correct positions in instrument rack on 07/24/2015. 

```

simulate_sequence.log
101) Sample      75      M2015-2192-1-BNBLK      Lab No.: M2015-2192-1
102) Sample      26      M2015-2192-1-BN        Lab No.: M2015-2192-1
103) Sample      74      M2015-2194-1-BNBLK      Lab No.: M2015-2194-1
104) Sample      27      M2015-2194-1-BN        Lab No.: M2015-2194-1
105) Sample      73      M2015-2243-1-BNBLK      Lab No.: M2015-2243-1
106) Sample      28      M2015-2243-1-BN        Lab No.: M2015-2243-1
107) Sample      72      M2015-2243-2-BNBLK      Lab No.: M2015-2243-2
108) Sample      29      M2015-2243-2-BN        Lab No.: M2015-2243-2
109) Sample      71      M2015-2417-2-BNBLK      Lab No.: M2015-2417-2
110) Sample      30      M2015-2417-2-BN        Lab No.: M2015-2417-2

```

```

Acquisition Method: GBT092509-Delta EMV.M
111) Sample      75      M2015-2192-1-BNBLKr     Lab No.: M2015-2192-1
112) Sample      26      M2015-2192-1-BNr        Lab No.: M2015-2192-1
113) Sample      74      M2015-2194-1-BNBLKr     Lab No.: M2015-2194-1
114) Sample      27      M2015-2194-1-BNr        Lab No.: M2015-2194-1
115) Sample      73      M2015-2243-1-BNBLKr     Lab No.: M2015-2243-1
116) Sample      28      M2015-2243-1-BNr        Lab No.: M2015-2243-1
117) Sample      72      M2015-2243-2-BNBLKr     Lab No.: M2015-2243-2
118) Sample      29      M2015-2243-2-BNr        Lab No.: M2015-2243-2
119) Sample      71      M2015-2417-2-BNBLKr     Lab No.: M2015-2417-2
120) Sample      30      M2015-2417-2-BNr        Lab No.: M2015-2417-2

```

```

Acquisition Method: BNSB120510.M
121) Sample      70      P2015-1534-1-BNBLK      Lab No.: P2015-1534-1
122) Sample      31      P2015-1534-1-BN        Lab No.: P2015-1534-1

```

```

Acquisition Method: GBT092509-Delta EMV.M
123) Sample      70      P2015-1534-1-BNBLKr     Lab No.: P2015-1534-1
124) Sample      31      P2015-1534-1-BNr        Lab No.: P2015-1534-1

```

```

Acquisition Method: BNSB120510.M
125) Sample      69      POSTBLKr                 BLK

```

```

Acquisition Method: GBT092509-Delta EMV.M
126) Sample      68      AFTER                     BLK
megabytes Needed: 2555 Space on drive D: 285762
Sequence Verification Done!

```

POC-AM 3.6.1-012425



Analytical Method 3.6.1 & 3.6.7 QA Check List

Run Start Date: 07/24/15

Analyst: DND

(Short GC/MS temperature program)

Positive Control Compound List




- Methamphetamine
- Nicotine
- Meperidine
- Caffeine
- Diphenhydramine
- Lidocaine
- PCP
- Methadone
- Amitriptyline
- Codeine
- Trazodone

Internal Standards

- Benzphetamine
- Papaverine


Optional back extraction **not** performed.
Samples reconstituted in methanol.

File :C:\gcms\1\data\Blood\072415\Prerun Solvent Blank.D
Operator : ISP\datastor
Acquired : 24 Jul 2015 11:41 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Pre-run Solvent Blank
Misc Info : Chloroform
Vial Number: 100

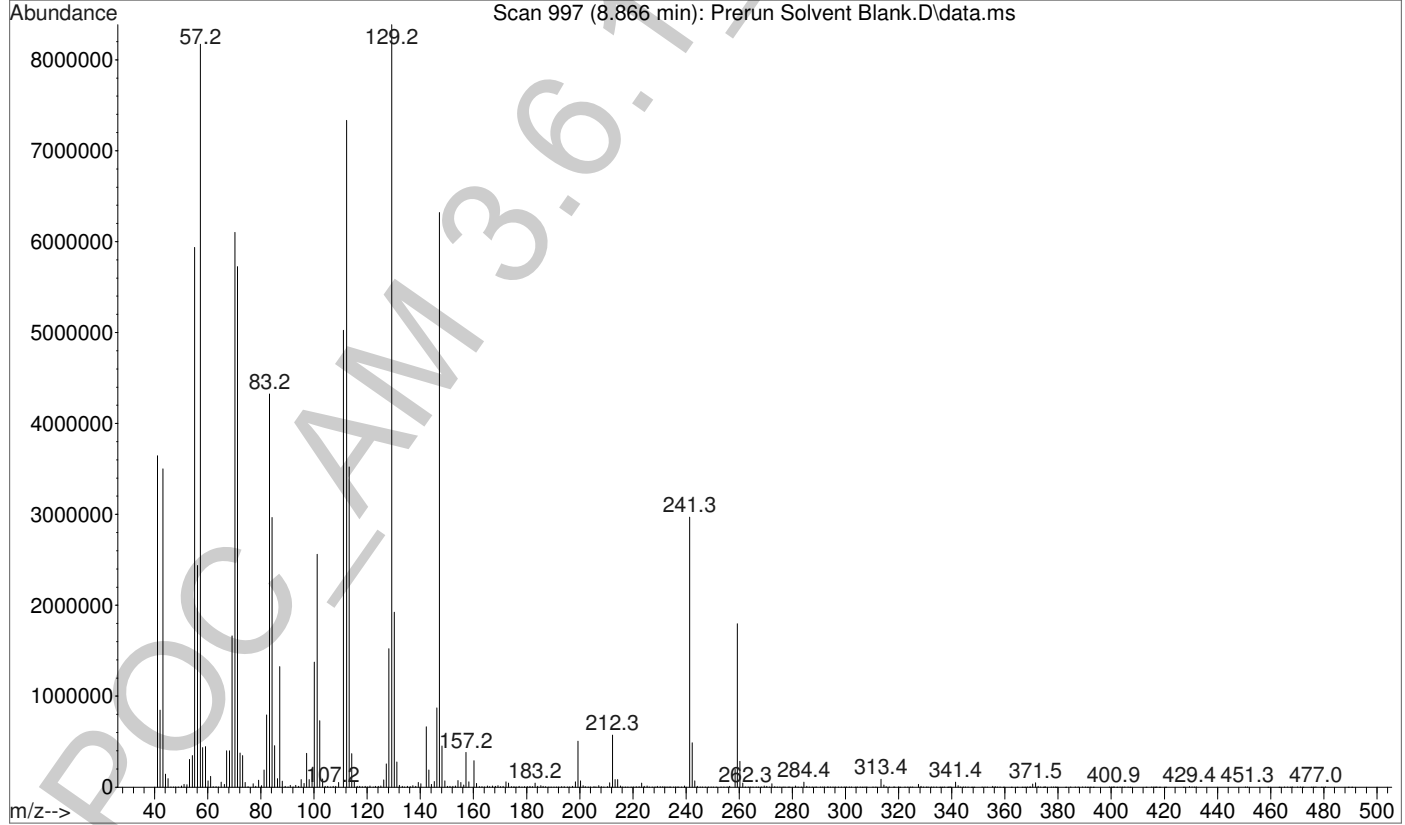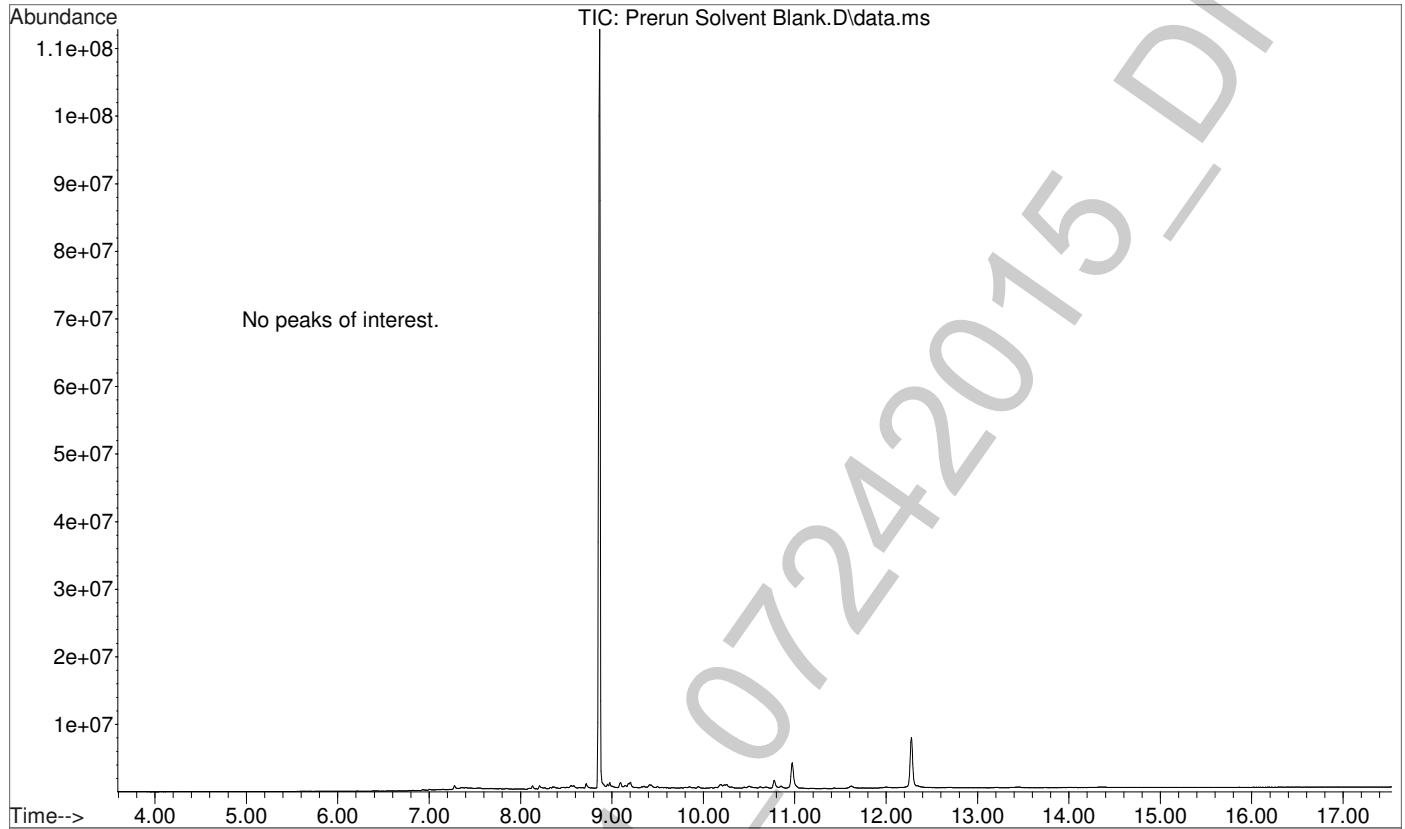







File :C:\gcms\1\data\Blood\072415\Negative Control-BN.D
Operator : ISP\datastor
Acquired : 24 Jul 2015 12:04 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1
Vial Number: 1

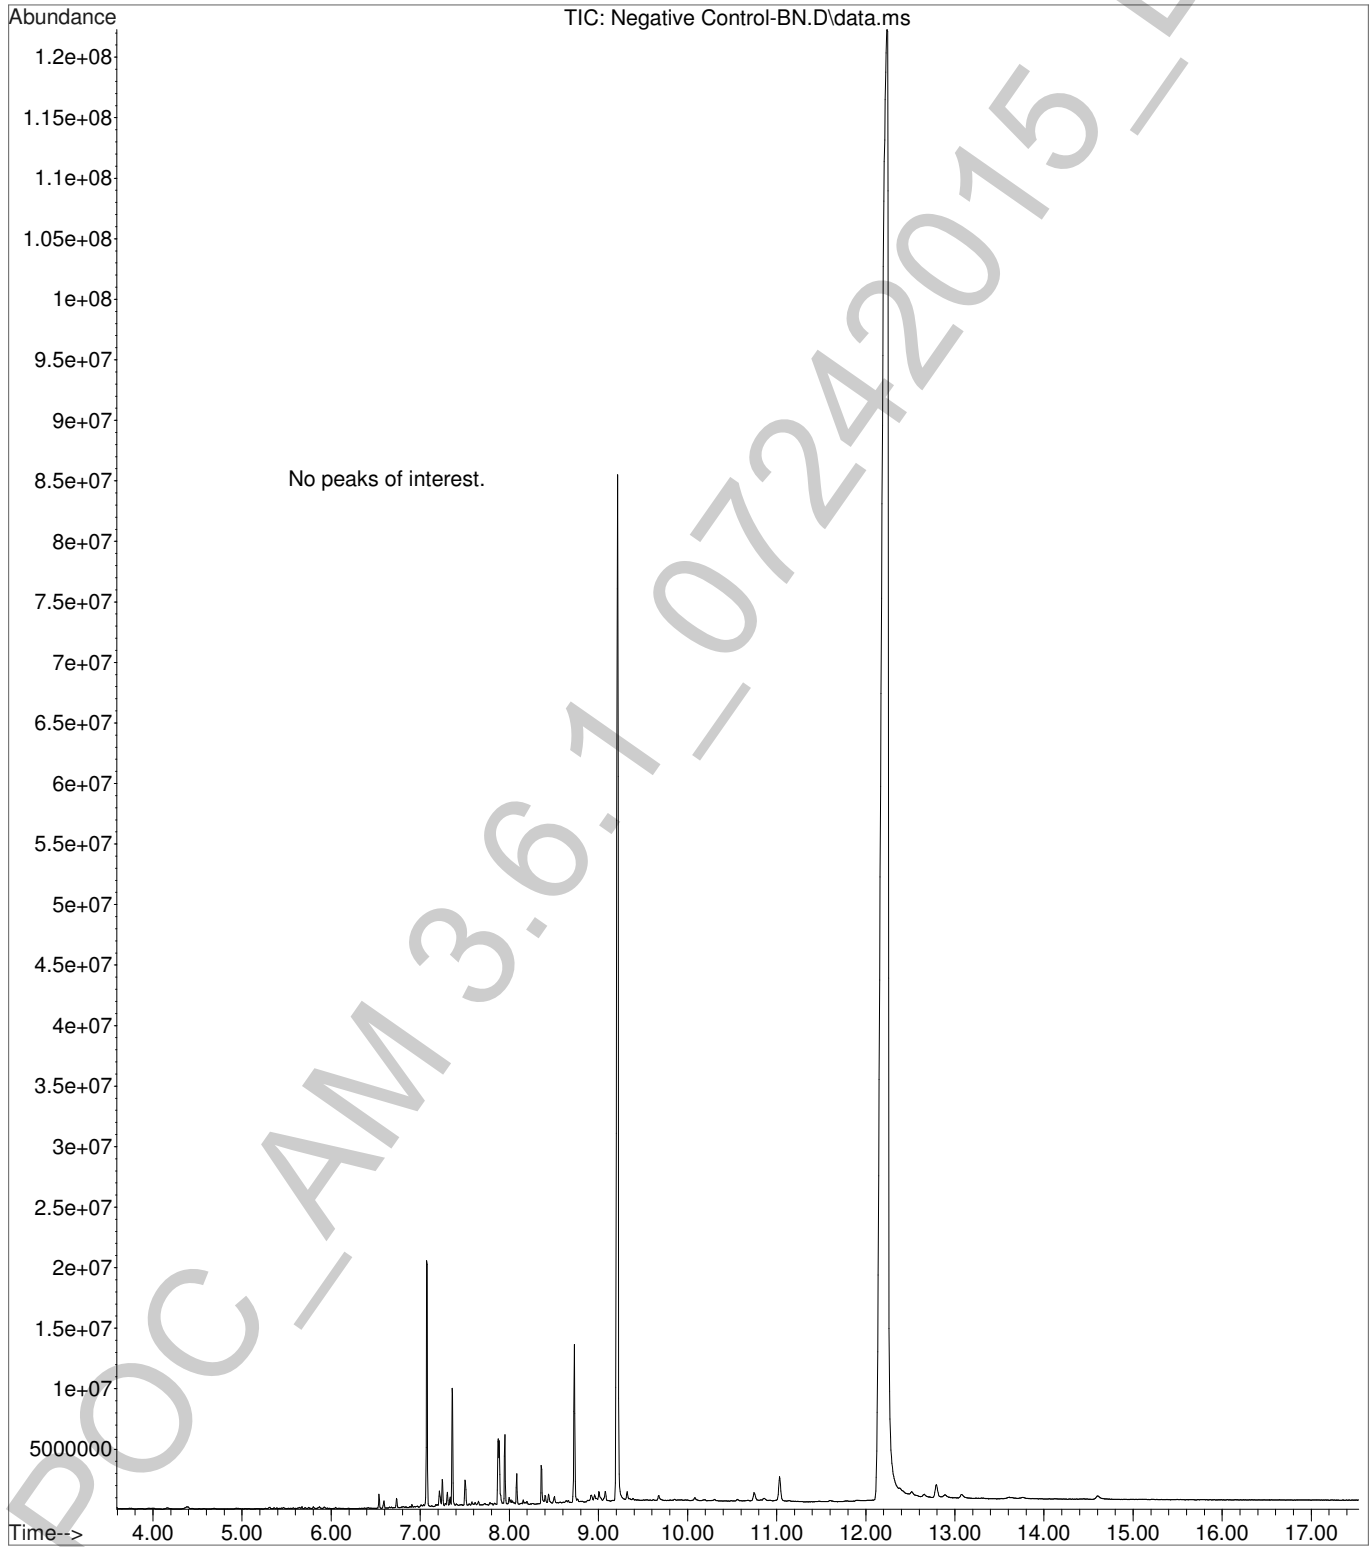

File :C:\gcms\1\data\Blood\072415\Negative Control-BN.D
Operator : ISP\datastor
Acquired : 24 Jul 2015 12:04 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1
Vial Number: 1

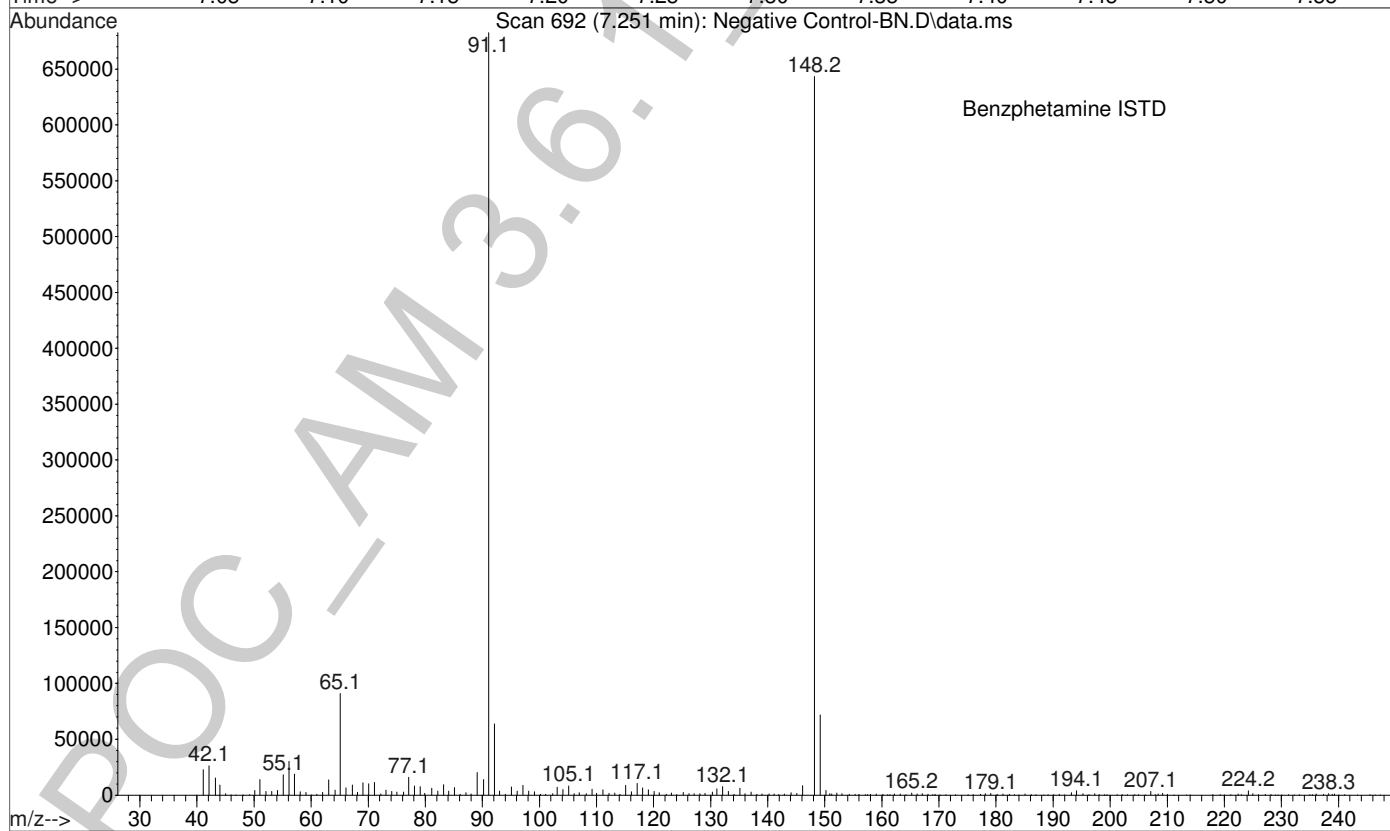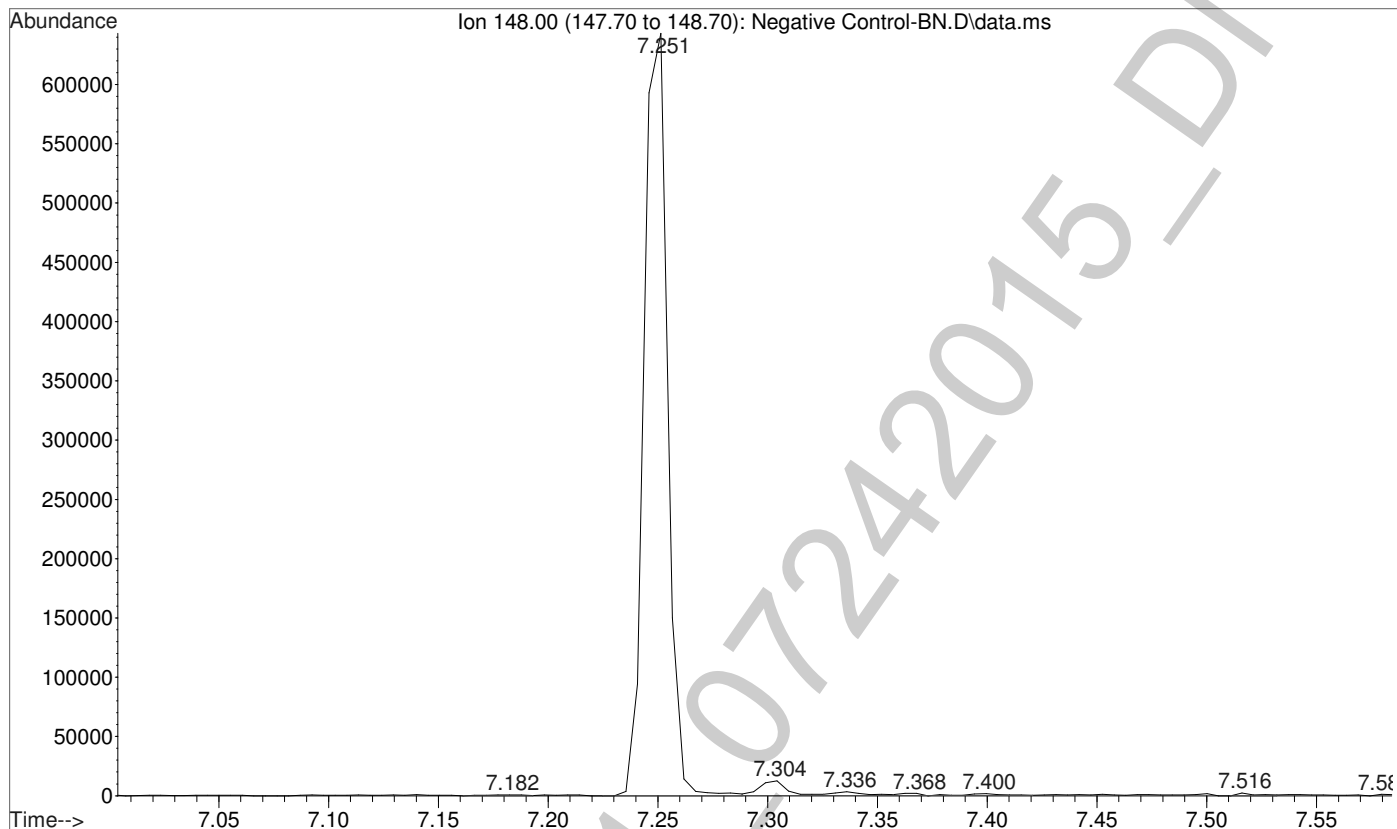


File :C:\gcms\1\data\Blood\072415\Negative Control-BN.D
Operator : ISP\datastor
Acquired : 24 Jul 2015 12:04 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1
Vial Number: 1

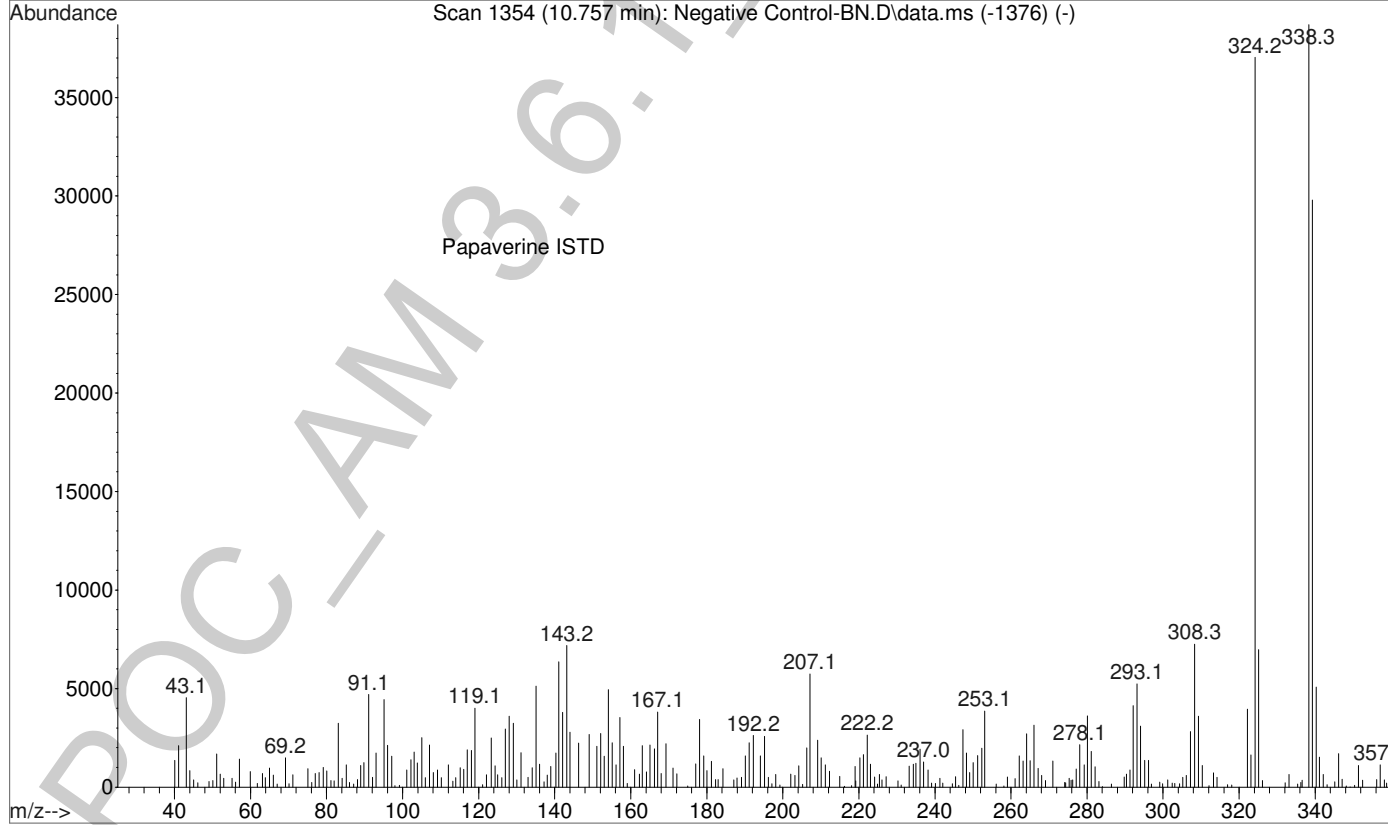
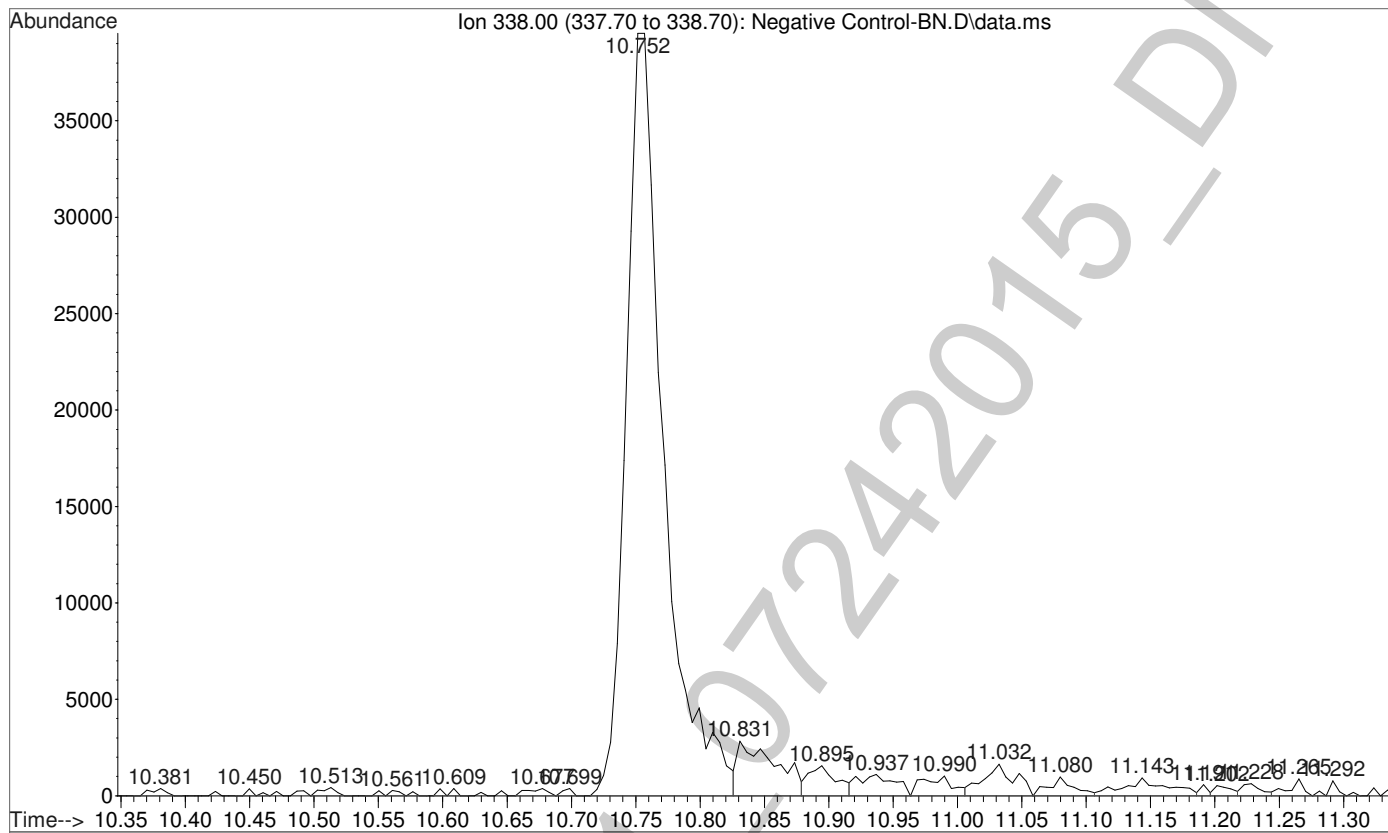






File :C:\gcms\1\data\Blood\072415\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 24 Jul 2015 12:27 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

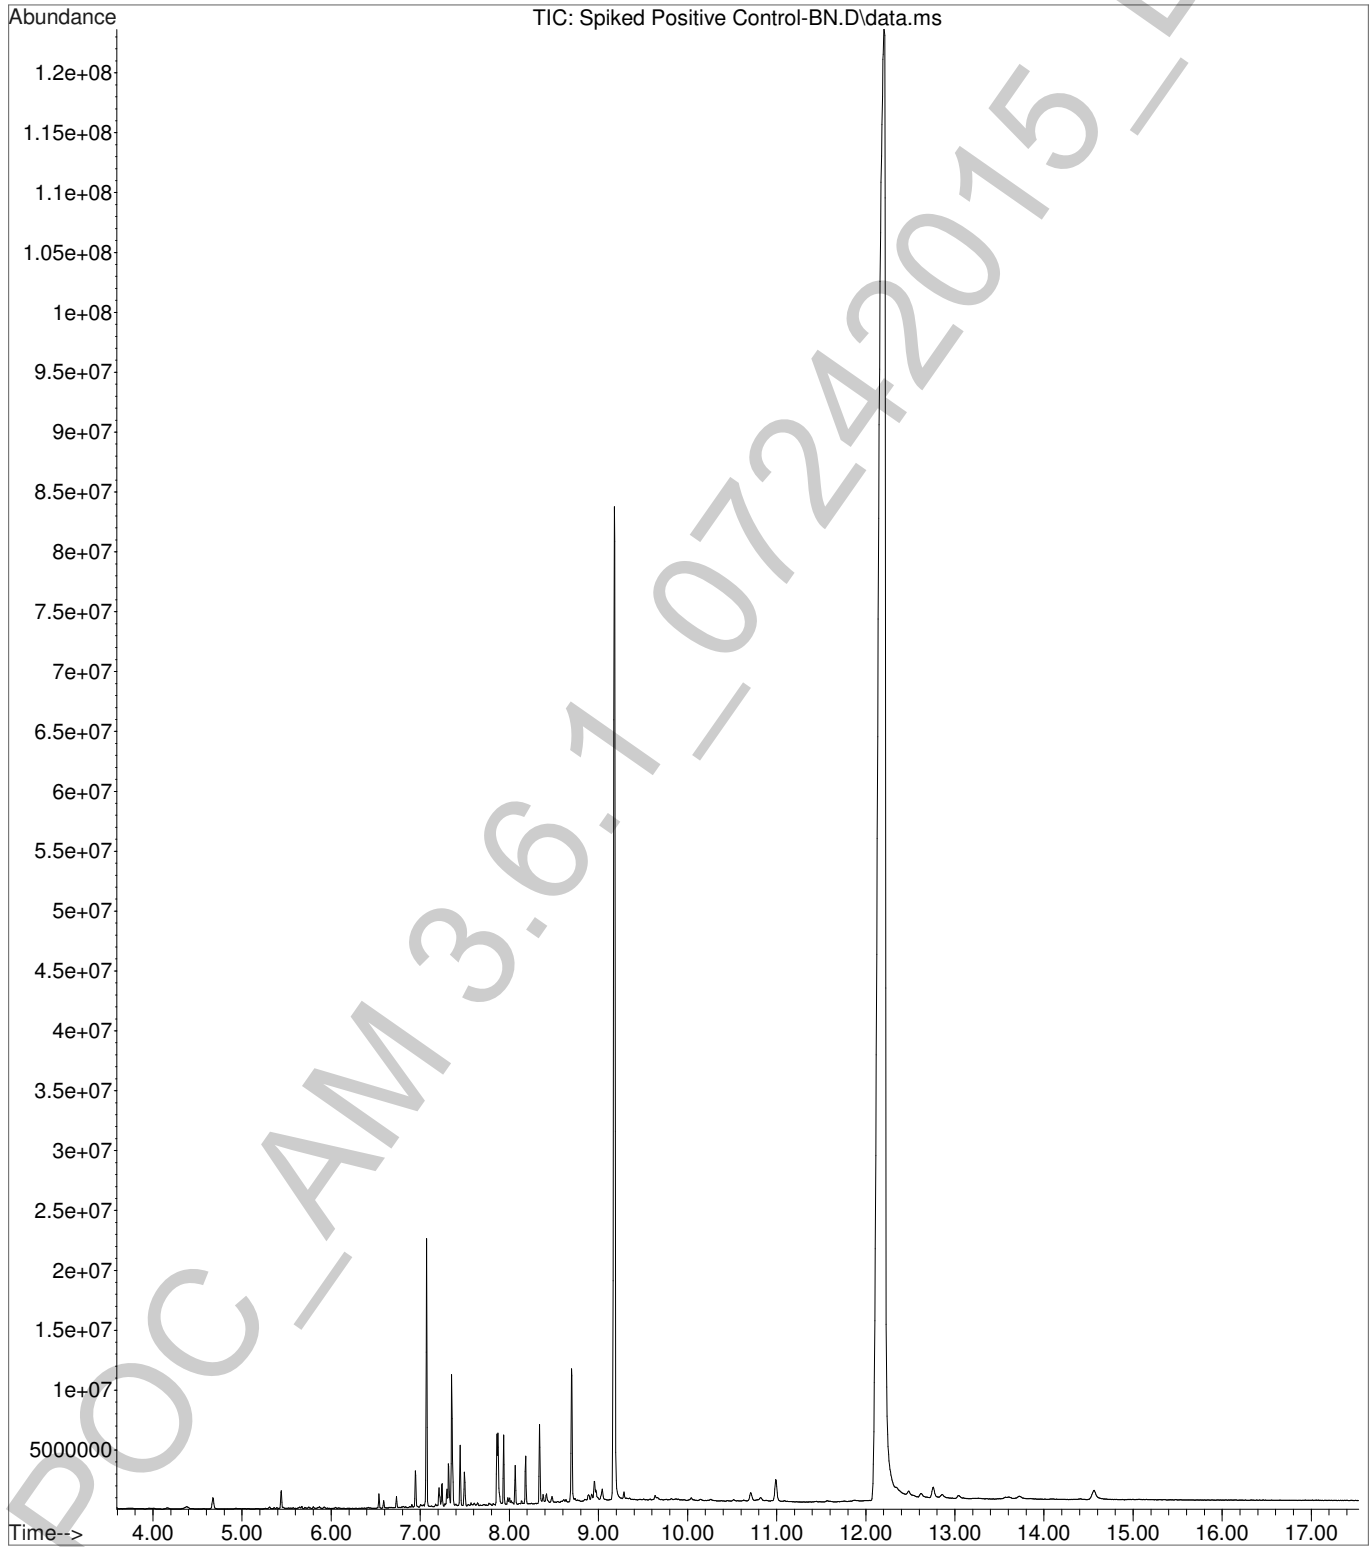



File :C:\gcms\1\data\Blood\072415\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 24 Jul 2015 12:27 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

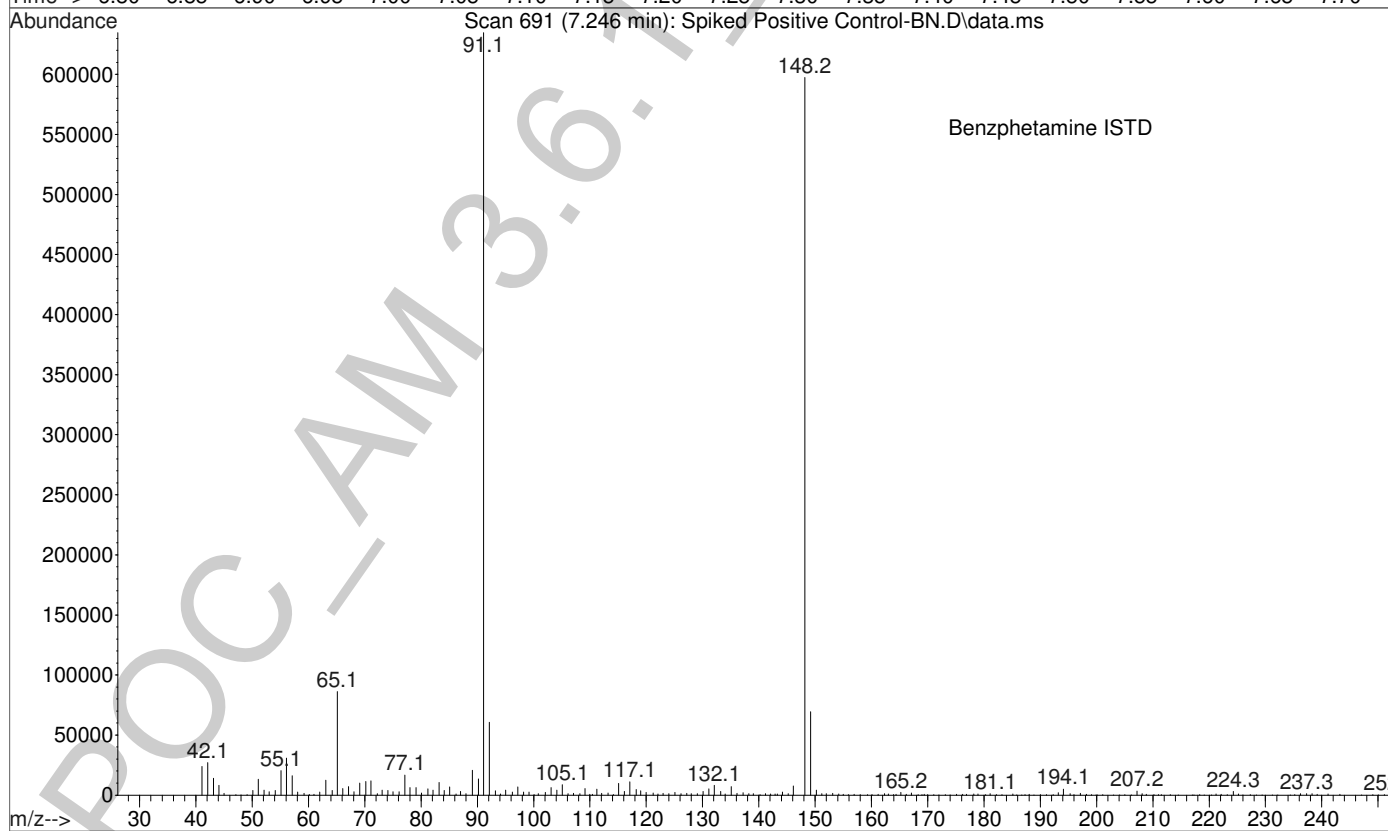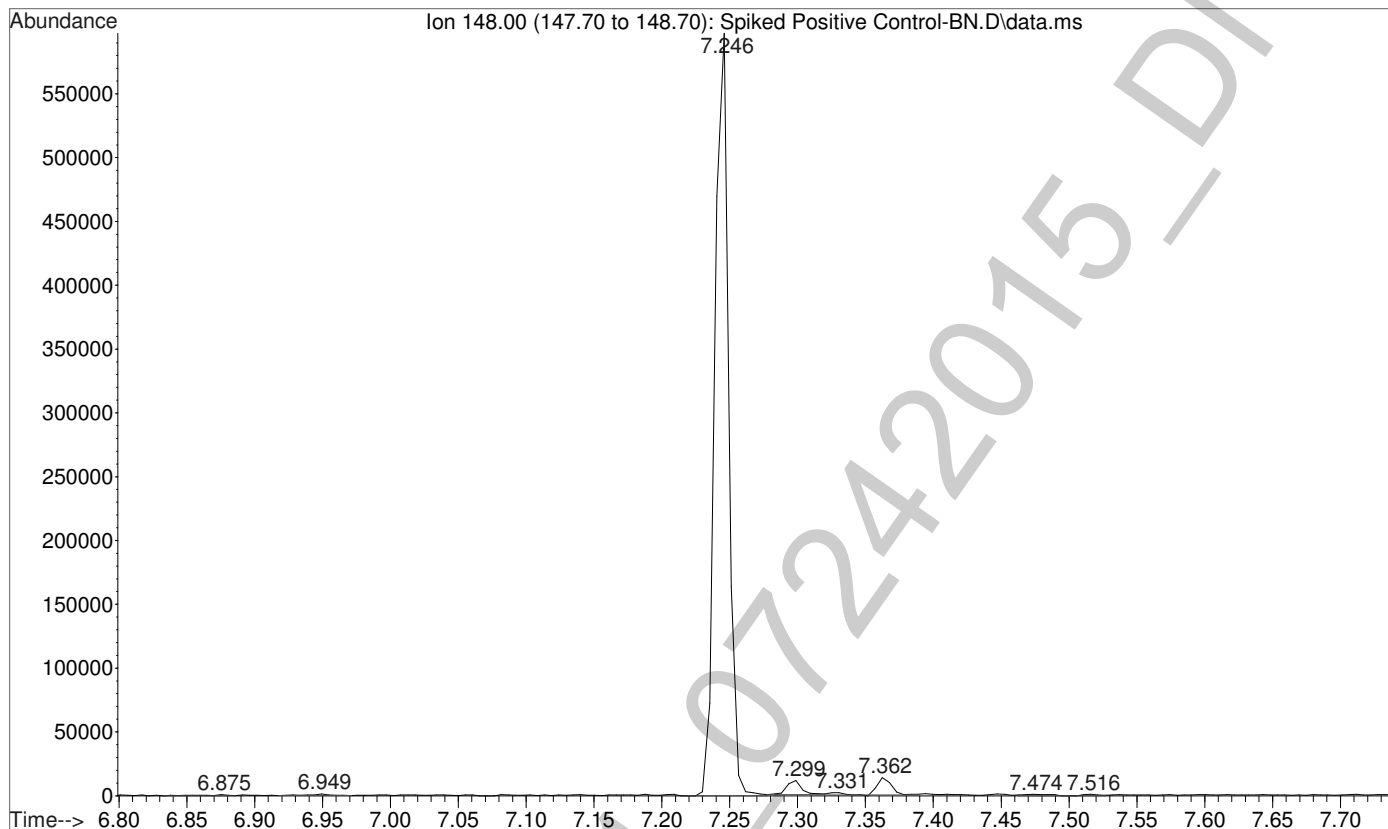



File :C:\gcms\1\data\Blood\072415\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 24 Jul 2015 12:27 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

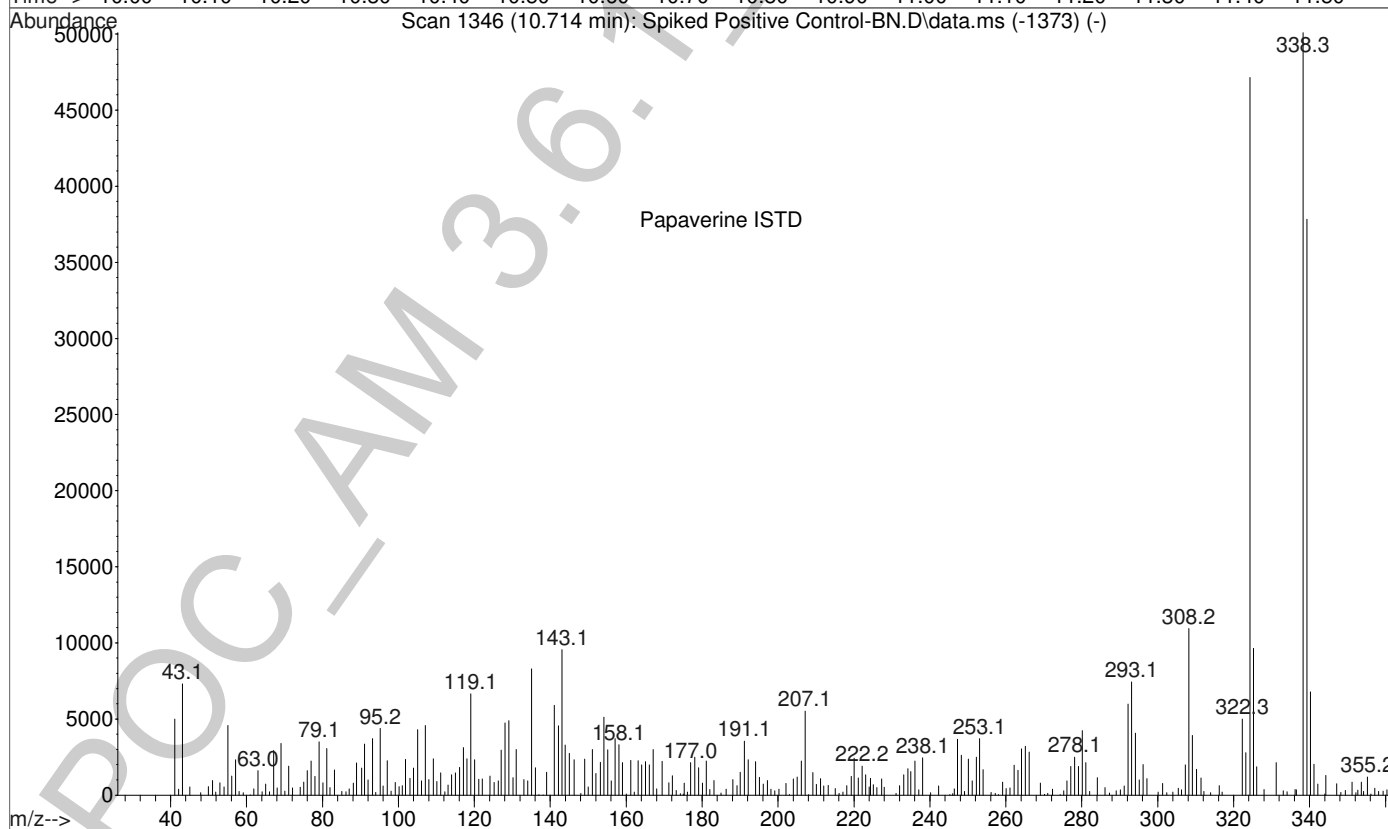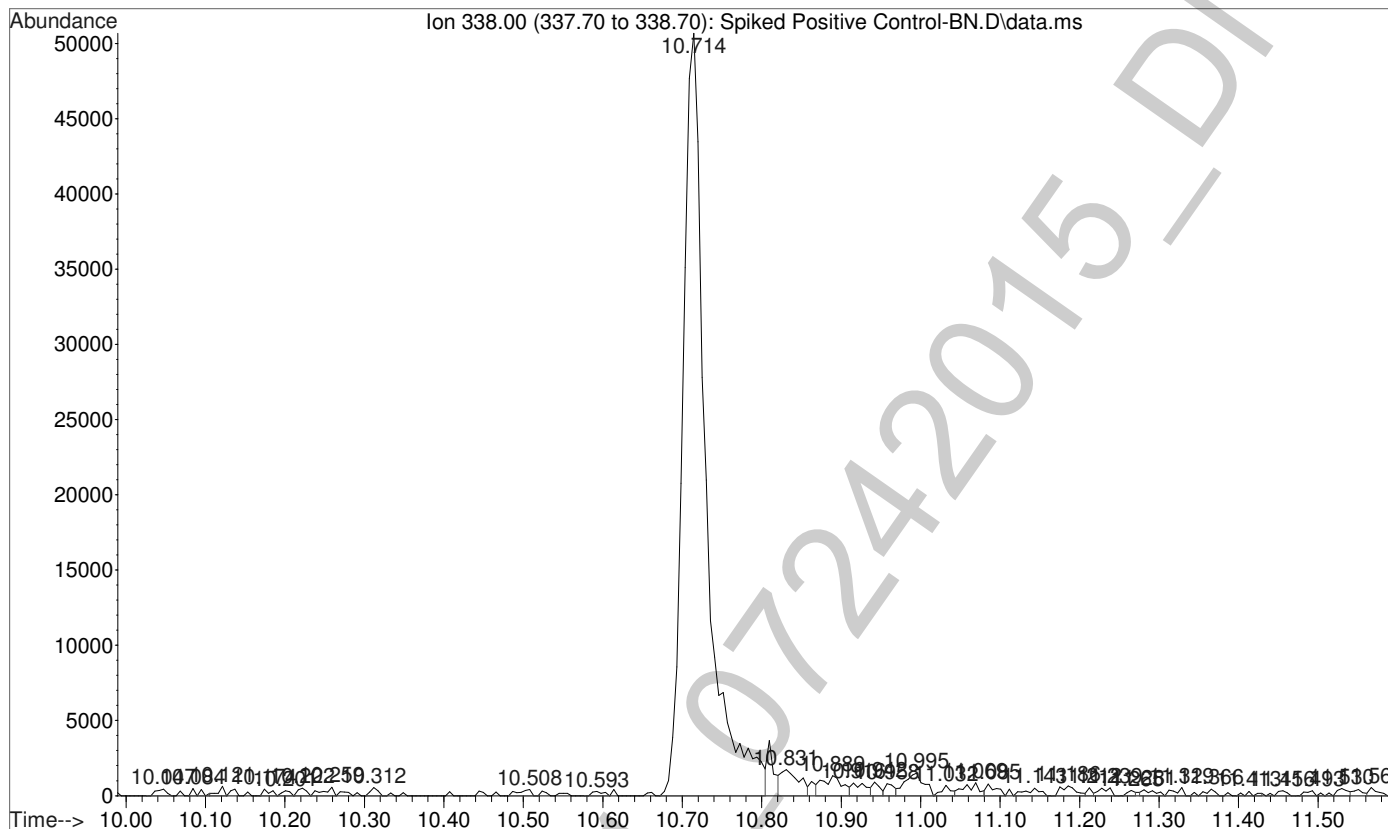



File :C:\gcms\1\data\Blood\072415\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 24 Jul 2015 12:27 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

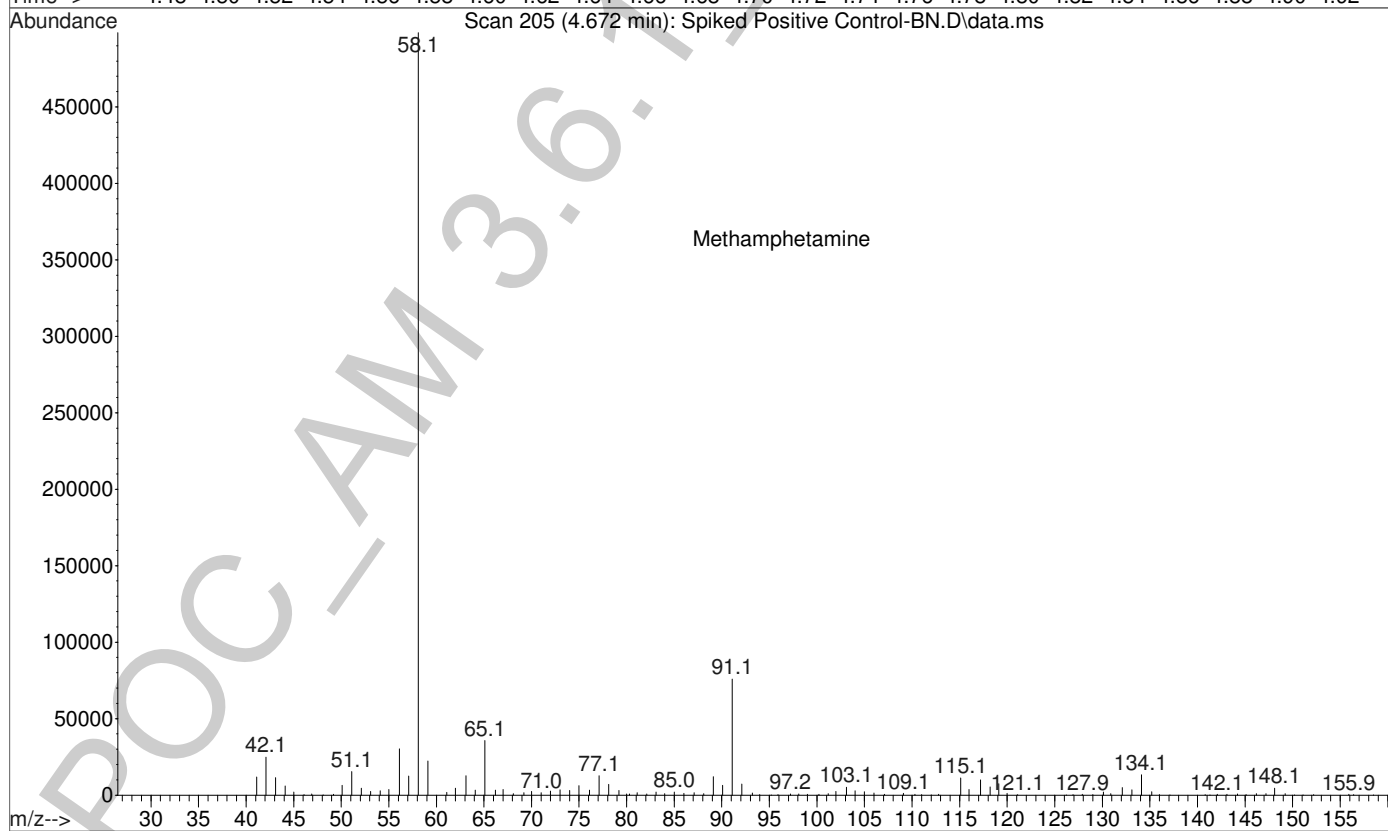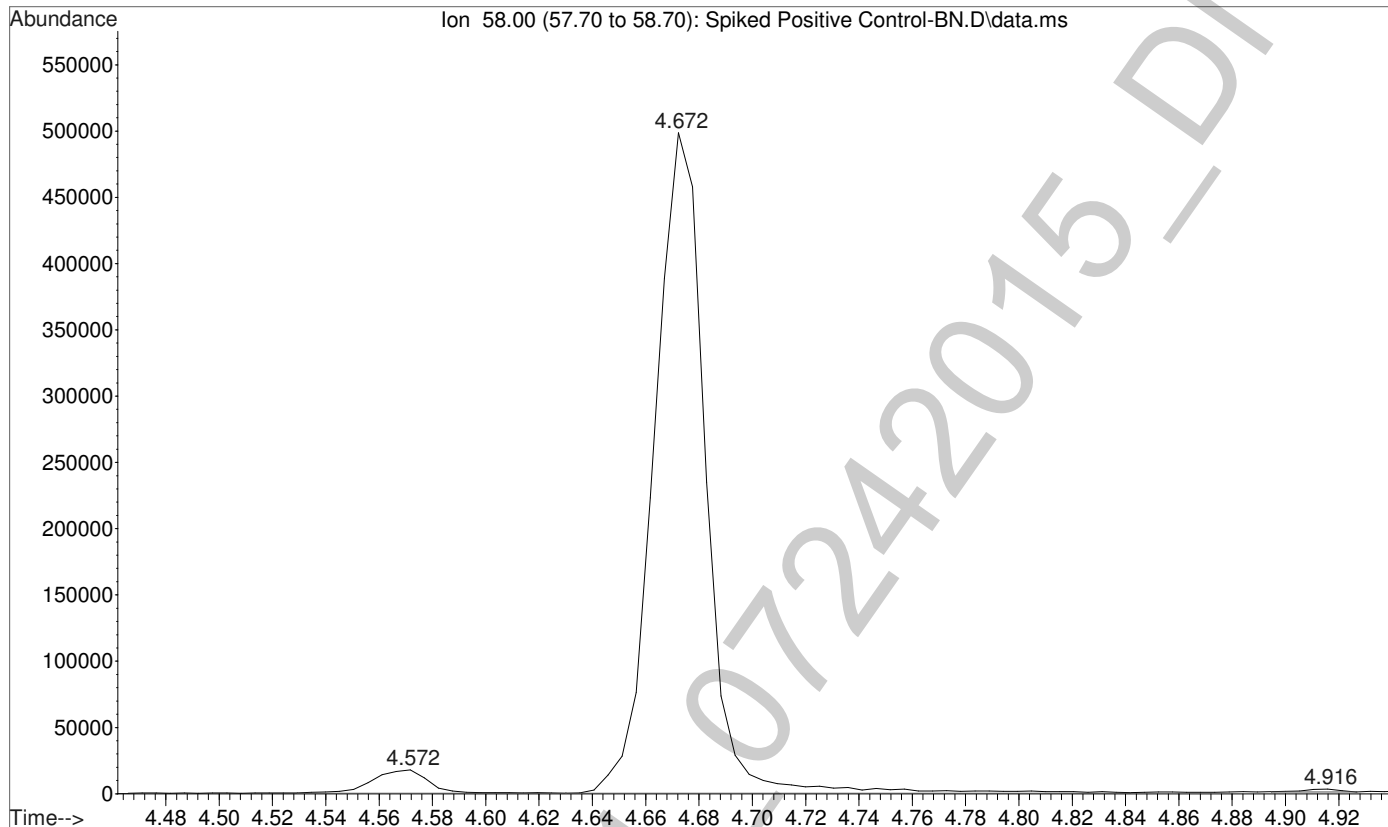



File :C:\gcms\1\data\Blood\072415\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 24 Jul 2015 12:27 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

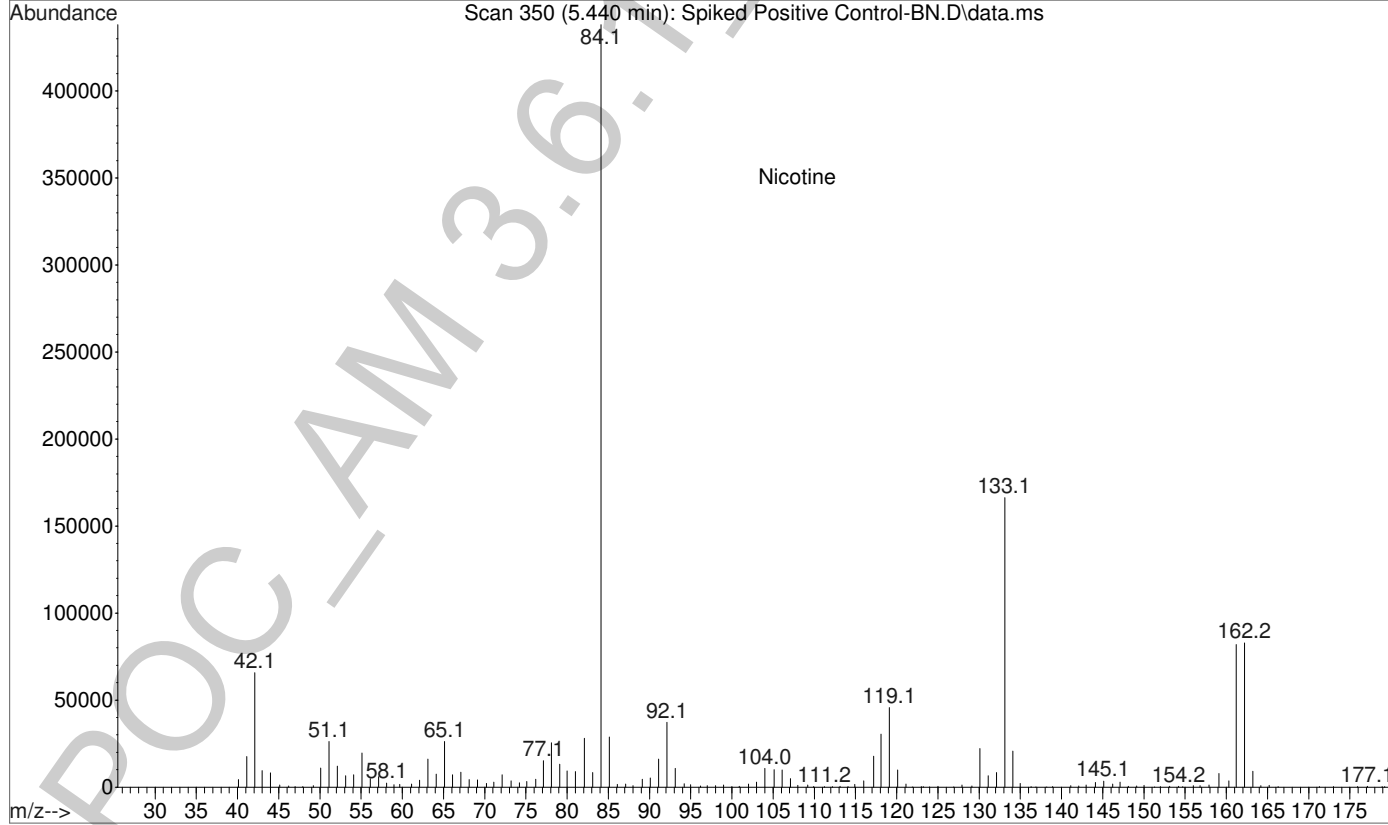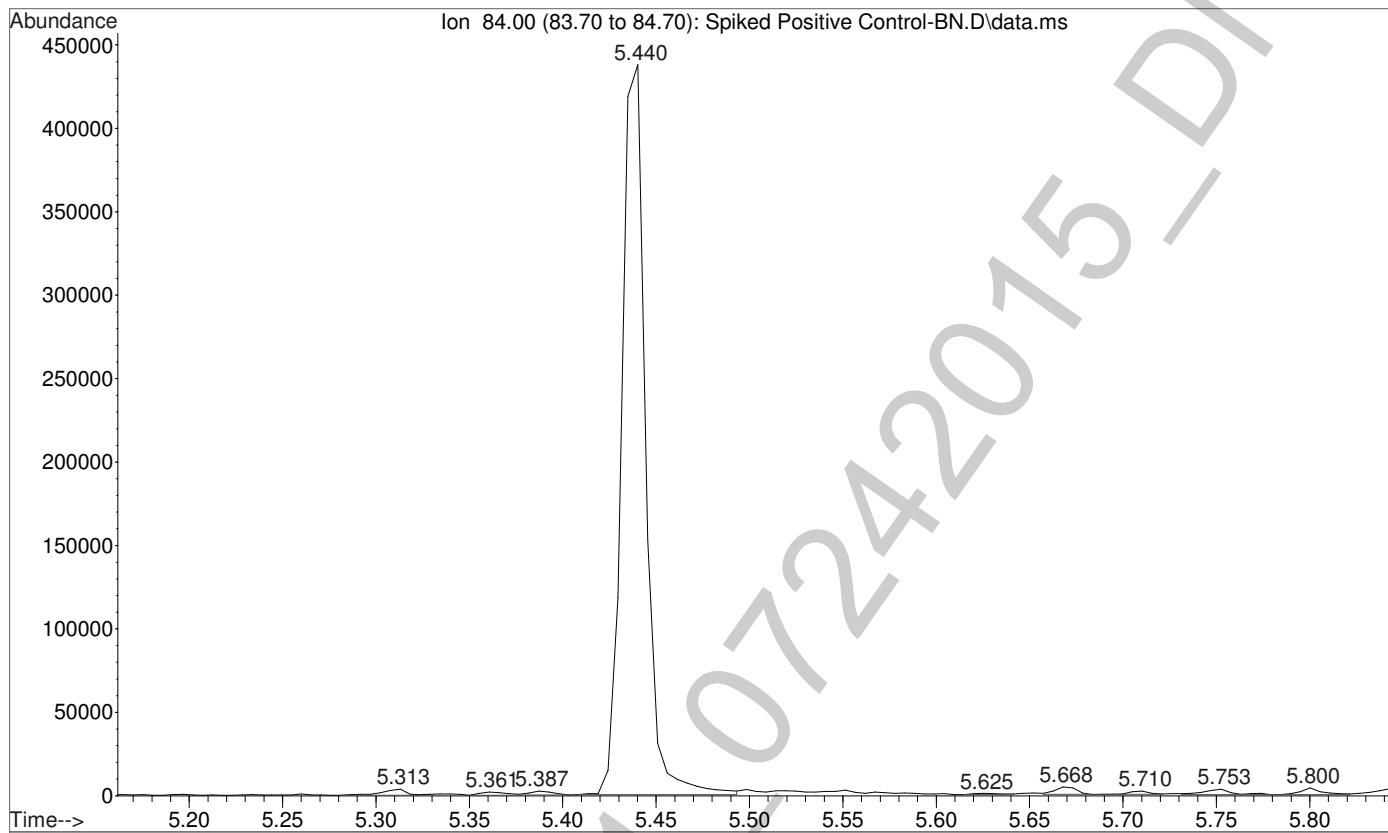



File :C:\gcms\1\data\Blood\072415\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 24 Jul 2015 12:27 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

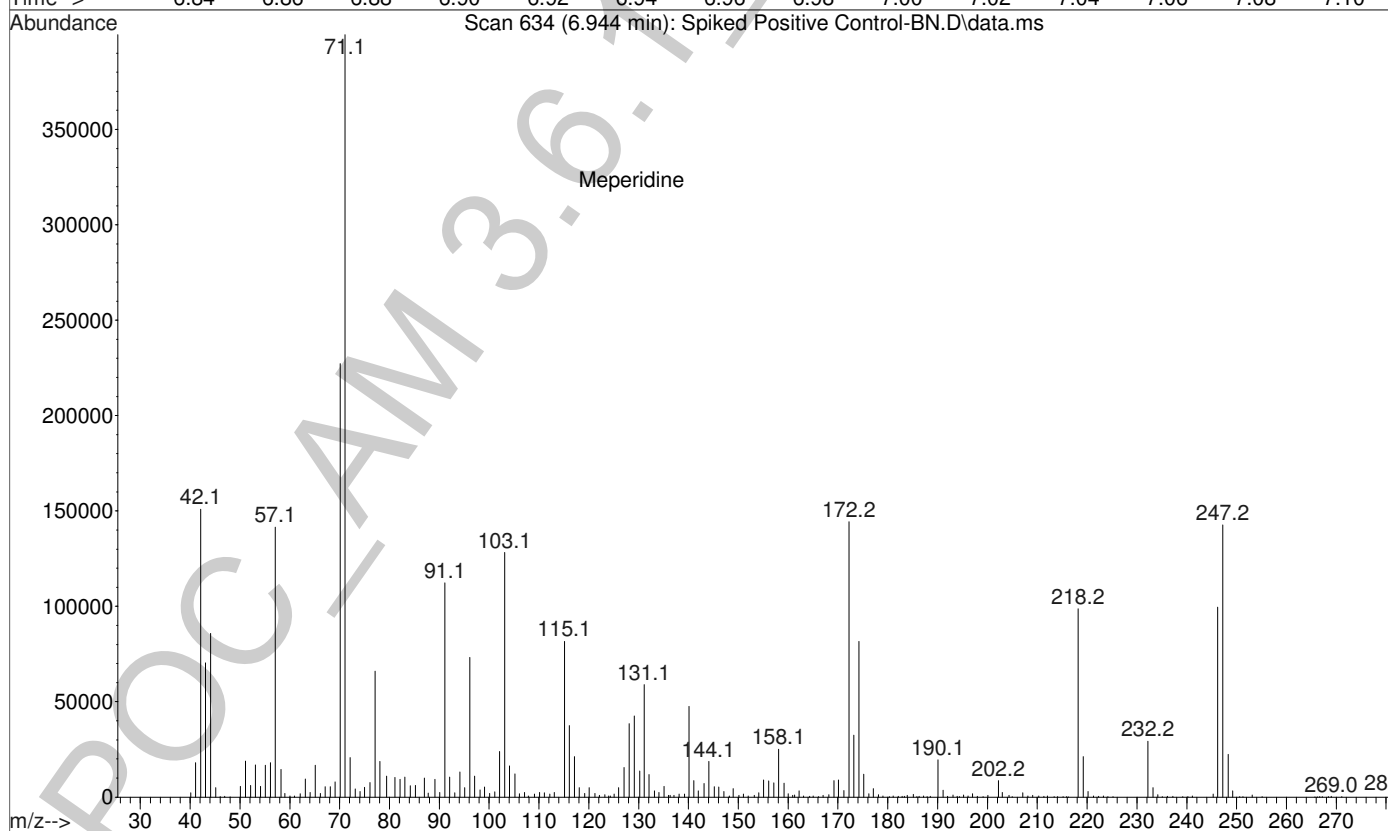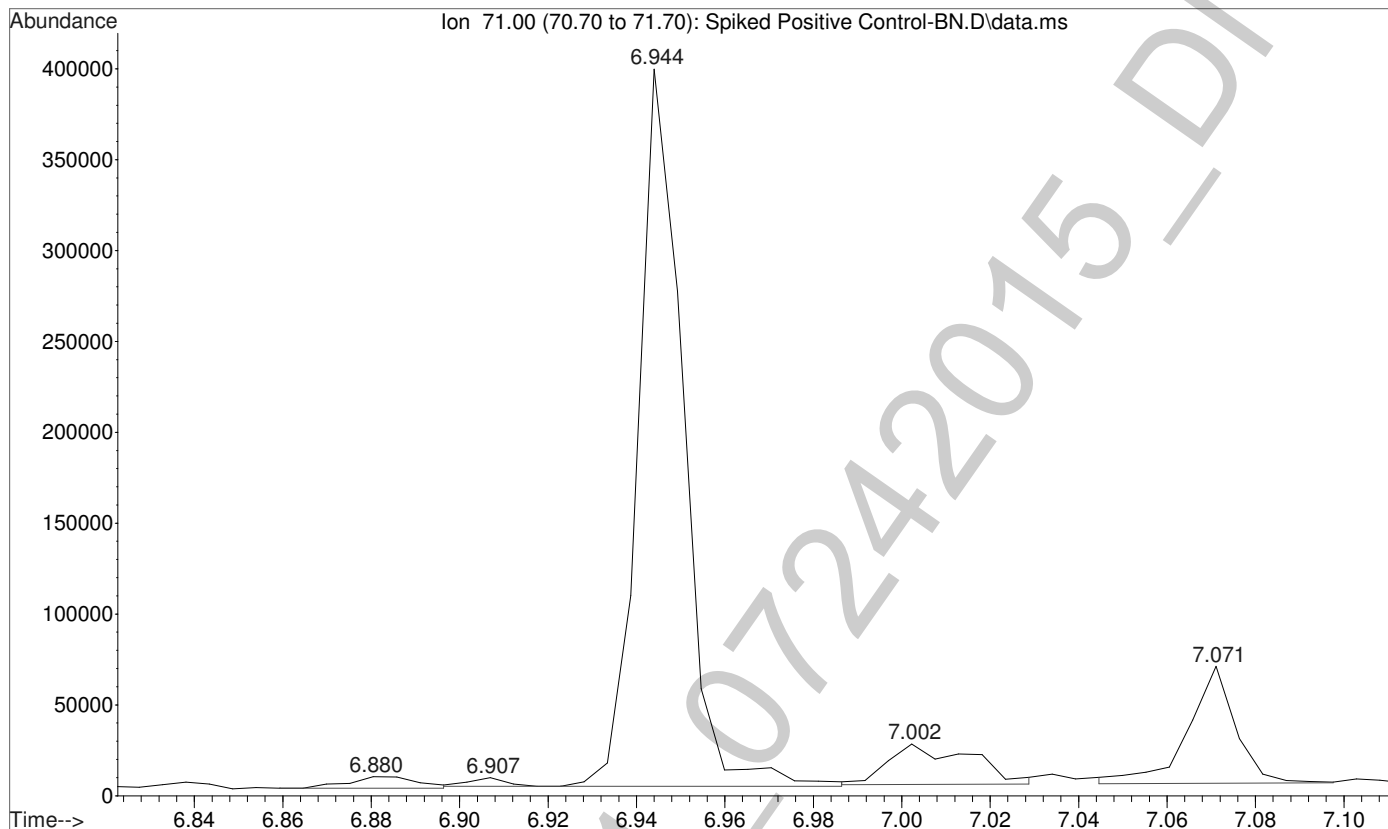



File :C:\gcms\1\data\Blood\072415\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 24 Jul 2015 12:27 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

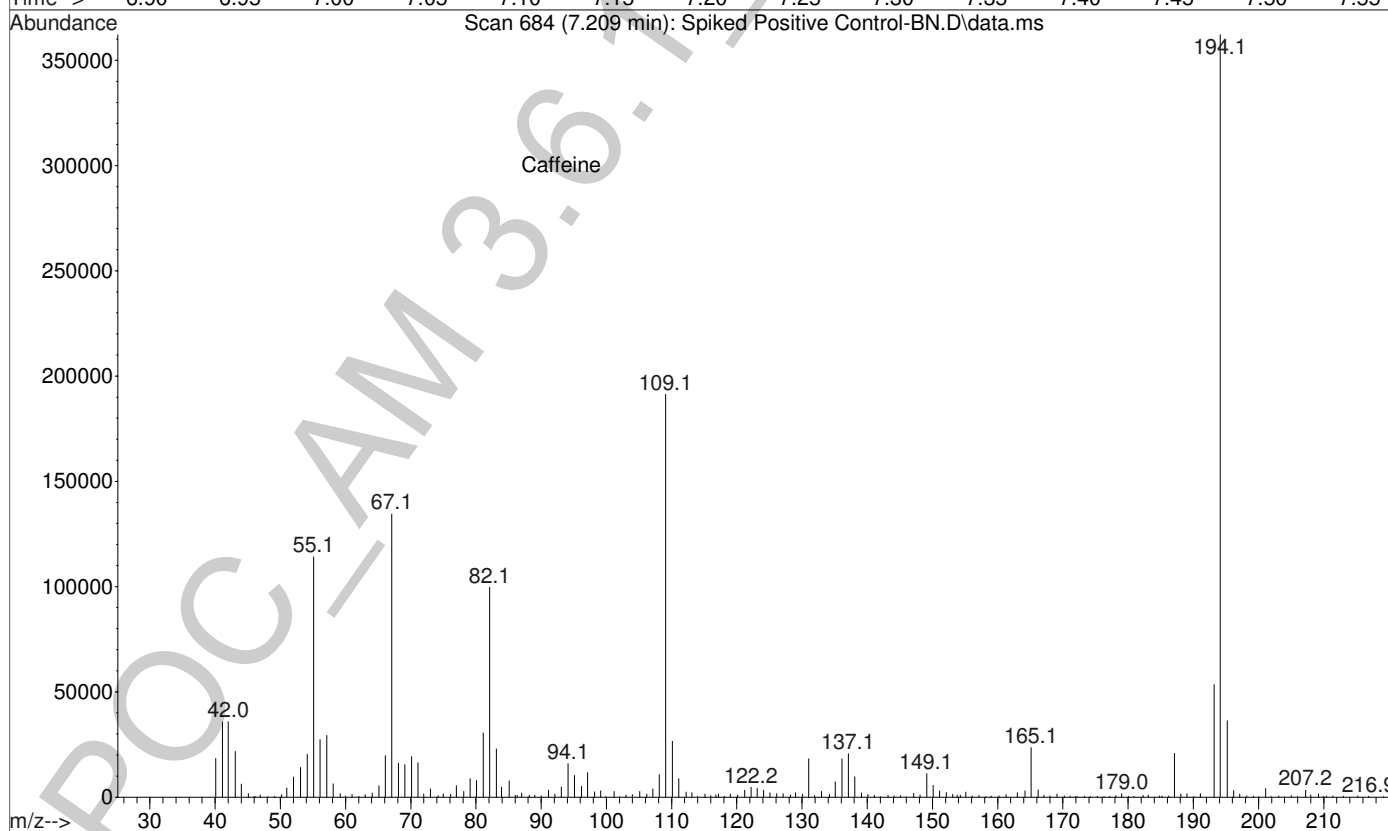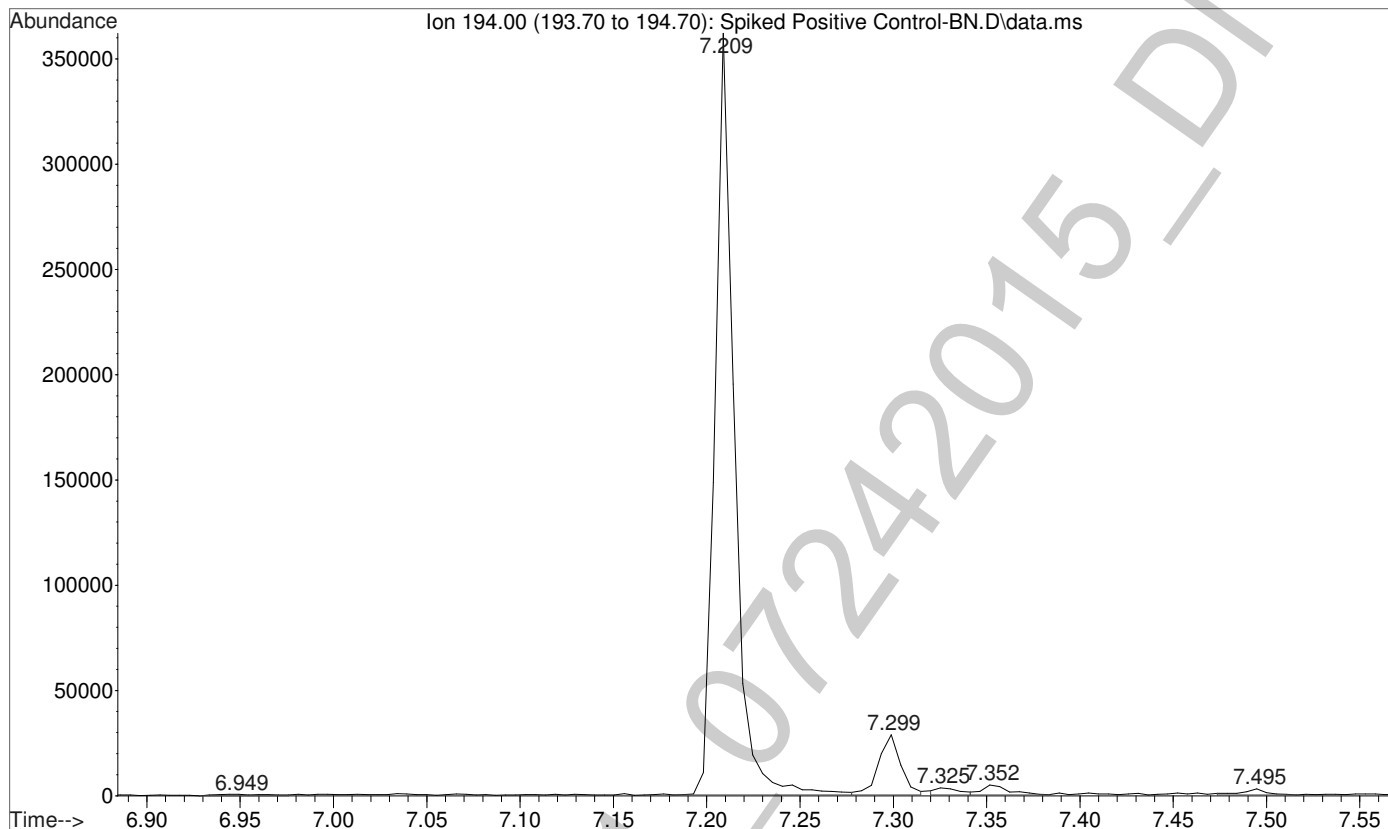



File :C:\gcms\1\data\Blood\072415\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 24 Jul 2015 12:27 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

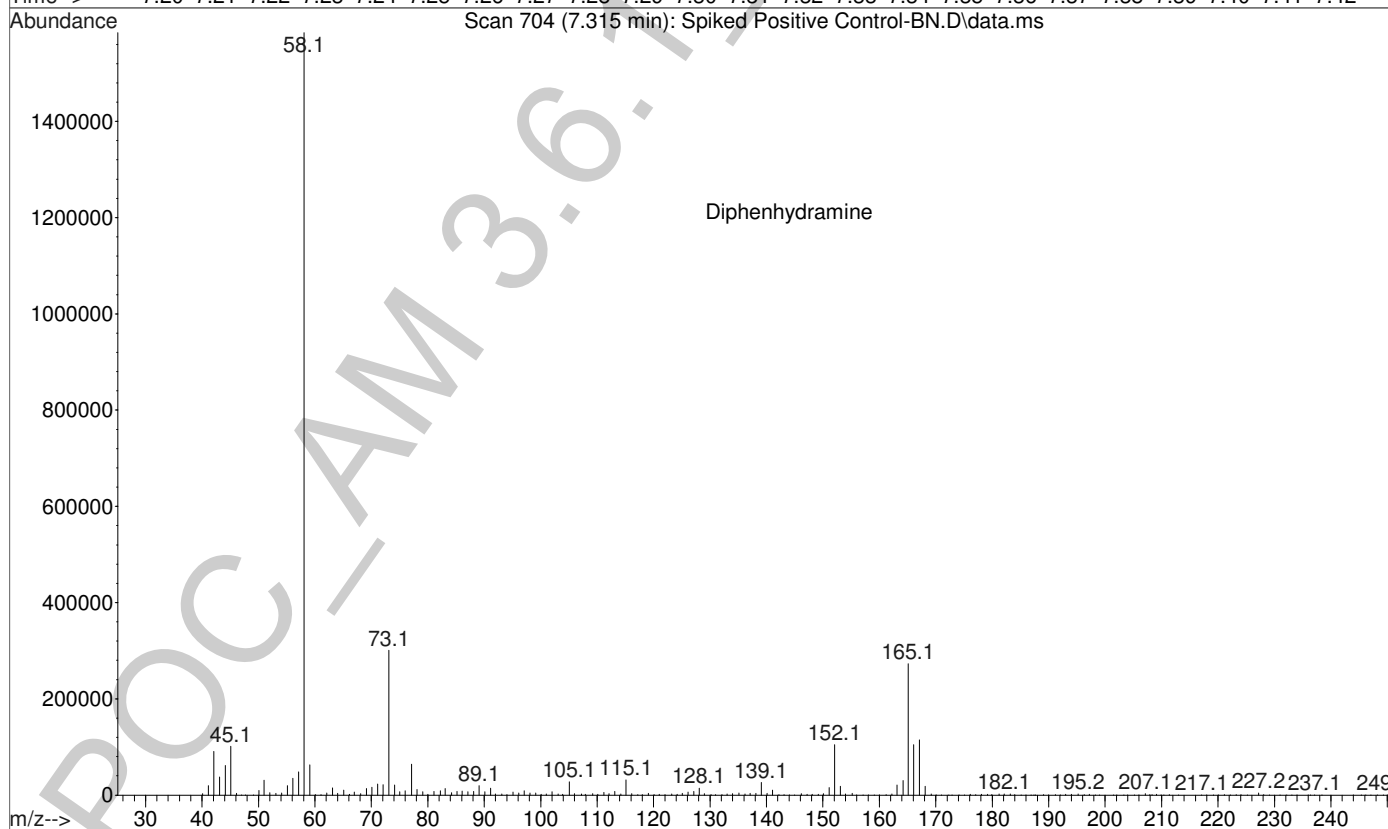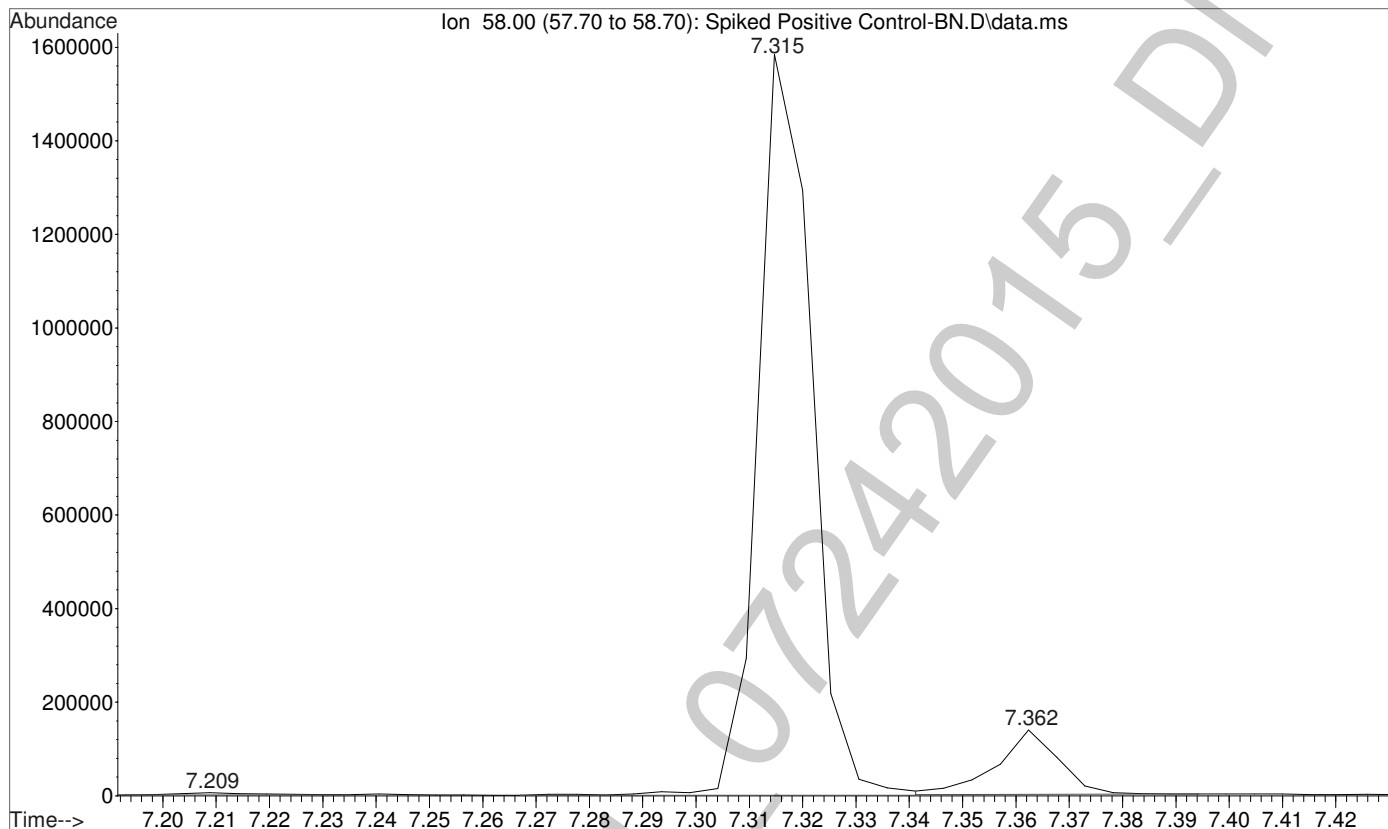



File :C:\gcms\1\data\Blood\072415\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 24 Jul 2015 12:27 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

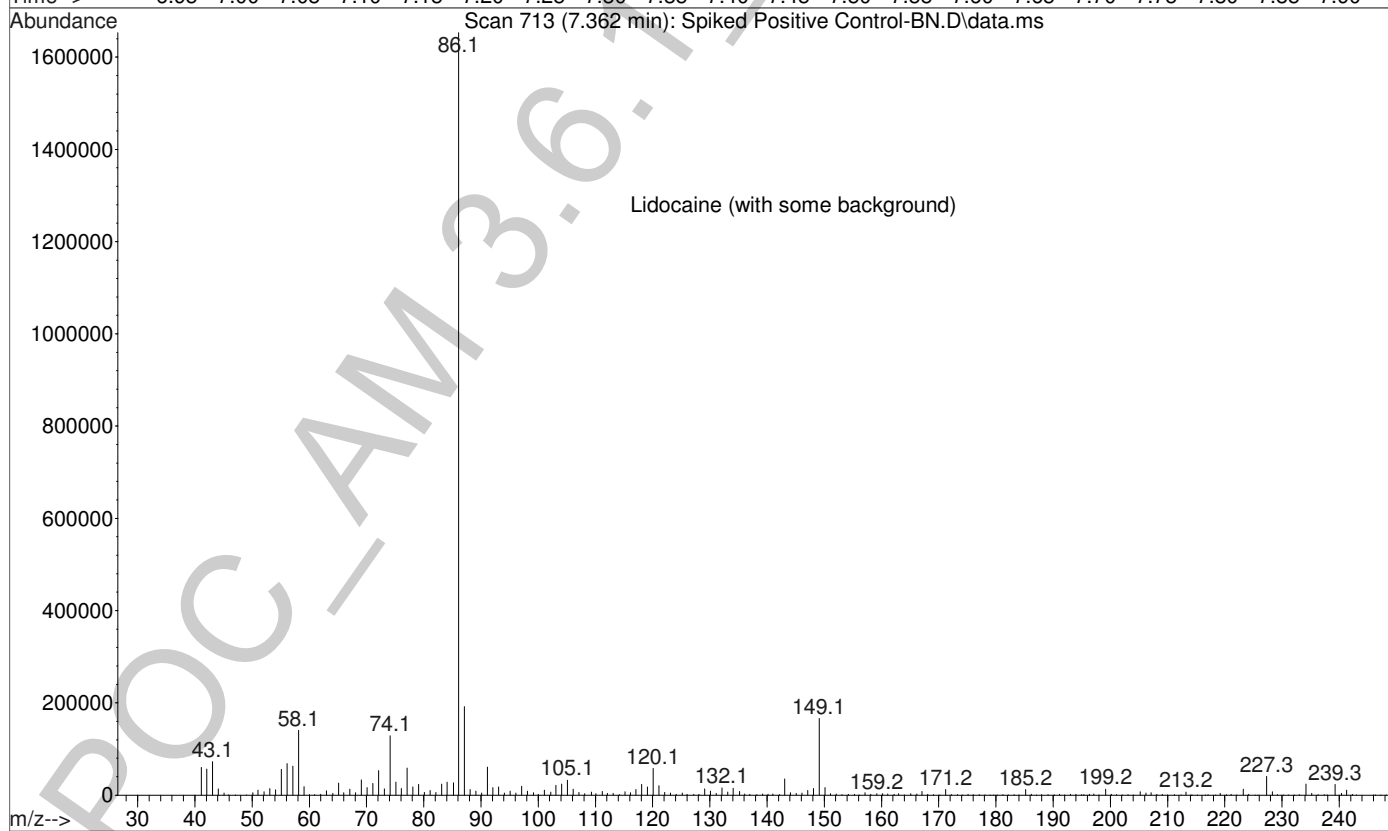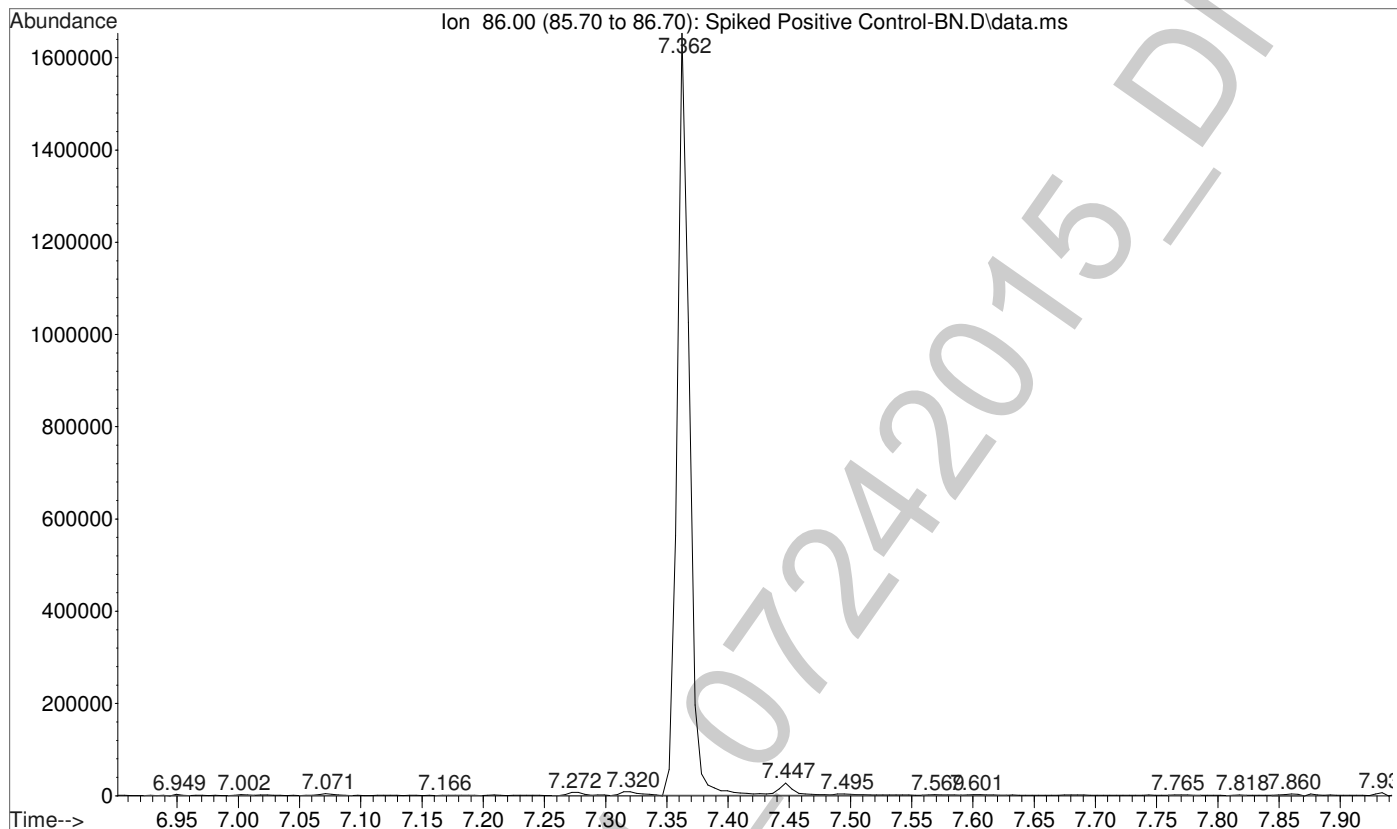



File :C:\gcms\1\data\Blood\072415\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 24 Jul 2015 12:27 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

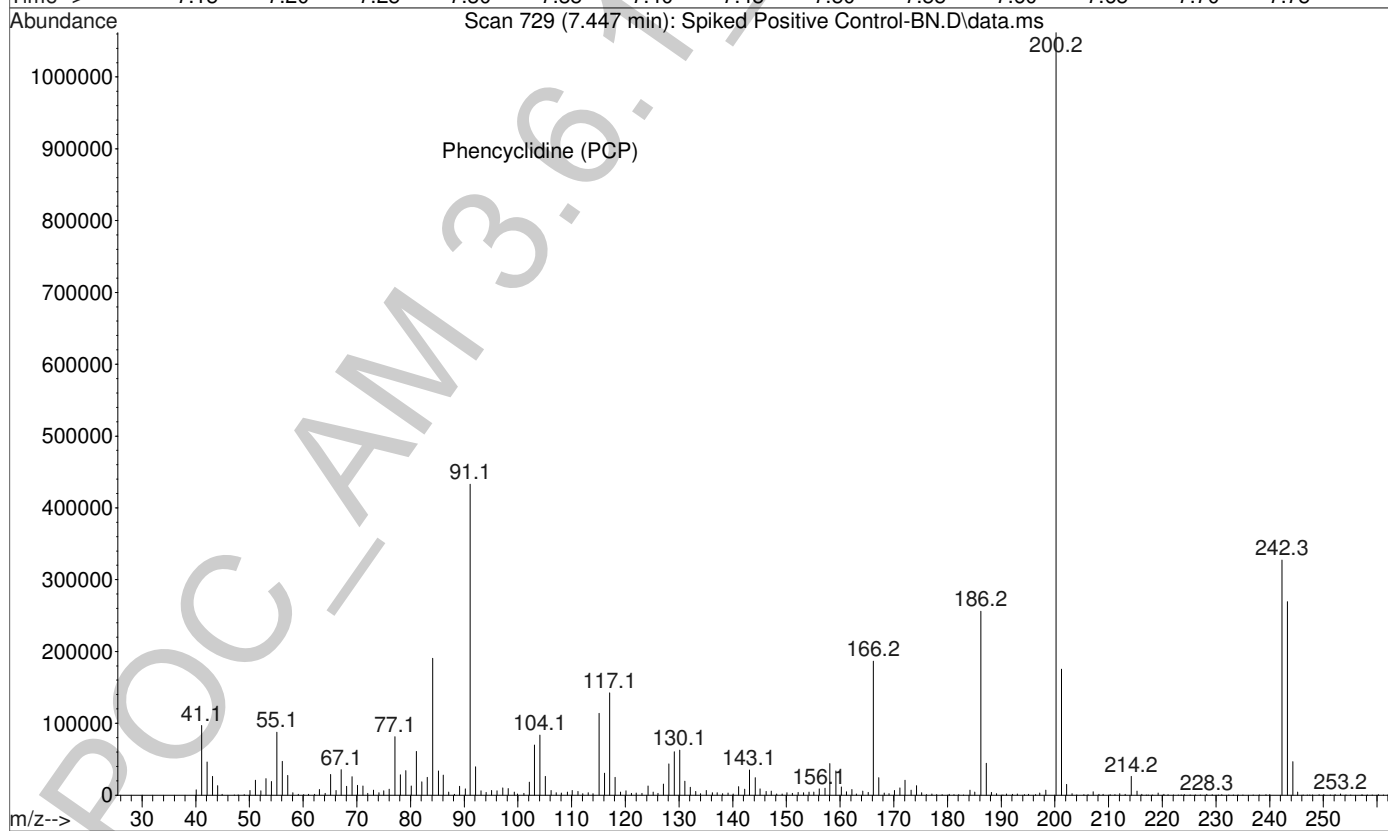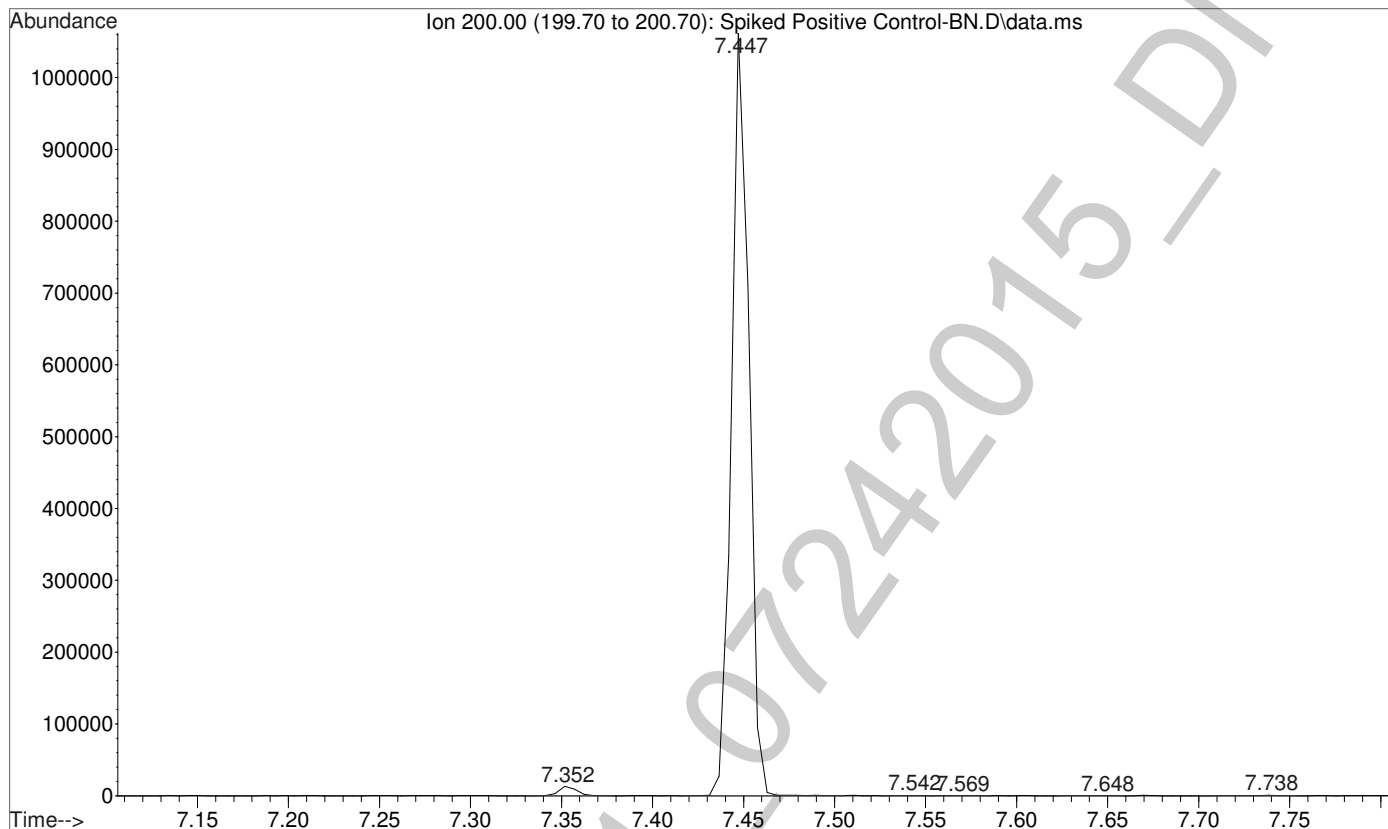



File :C:\gcms\1\data\Blood\072415\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 24 Jul 2015 12:27 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

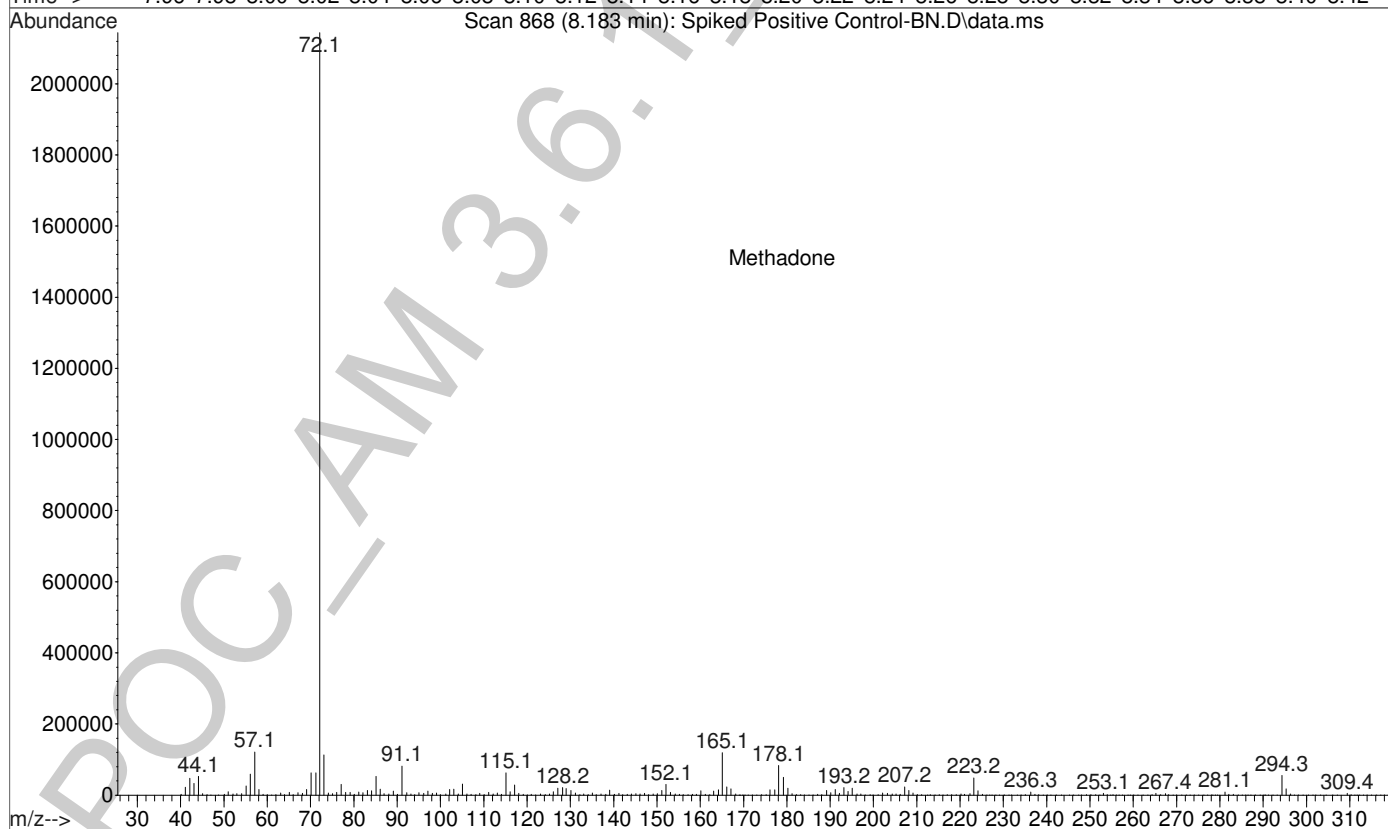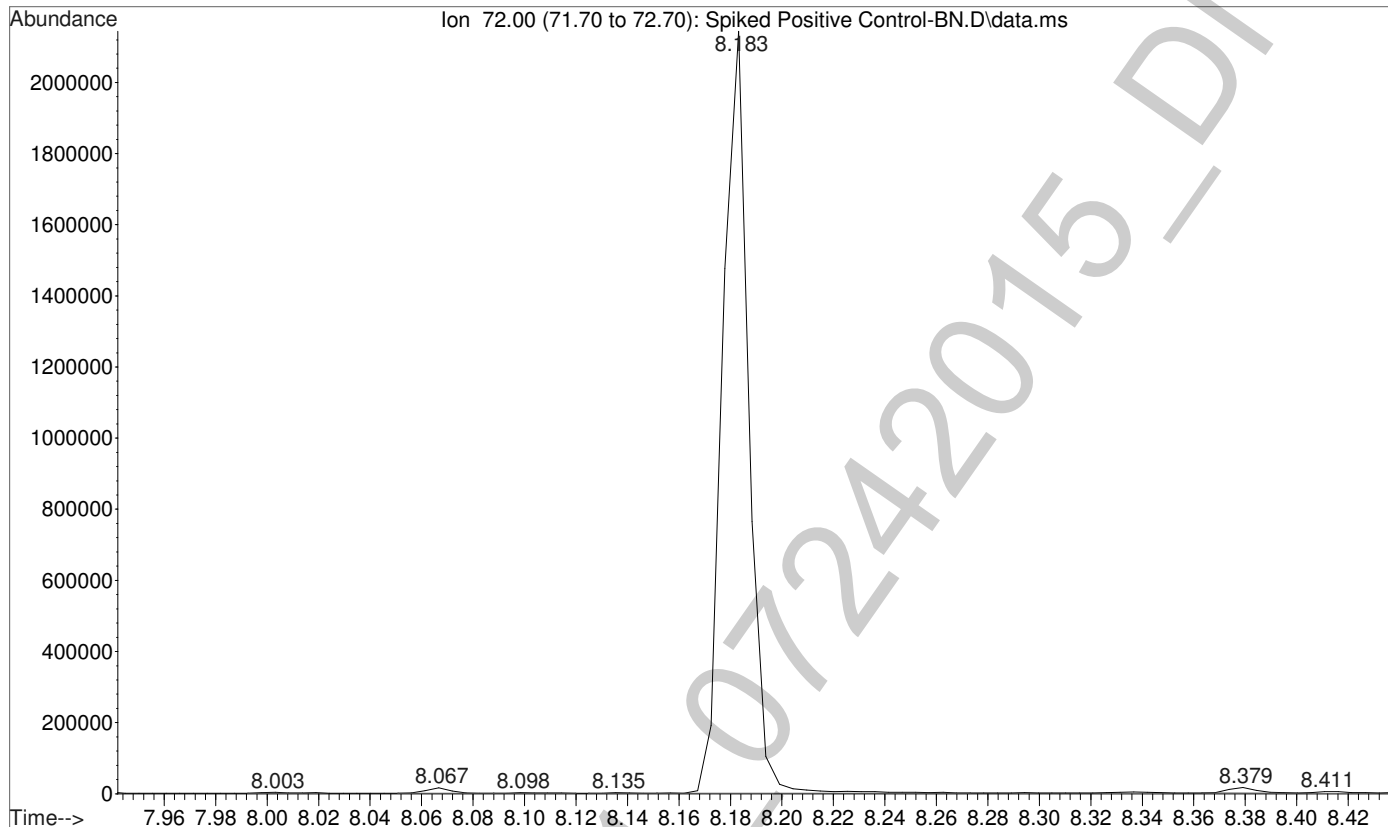



File :C:\gcms\1\data\Blood\072415\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 24 Jul 2015 12:27 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

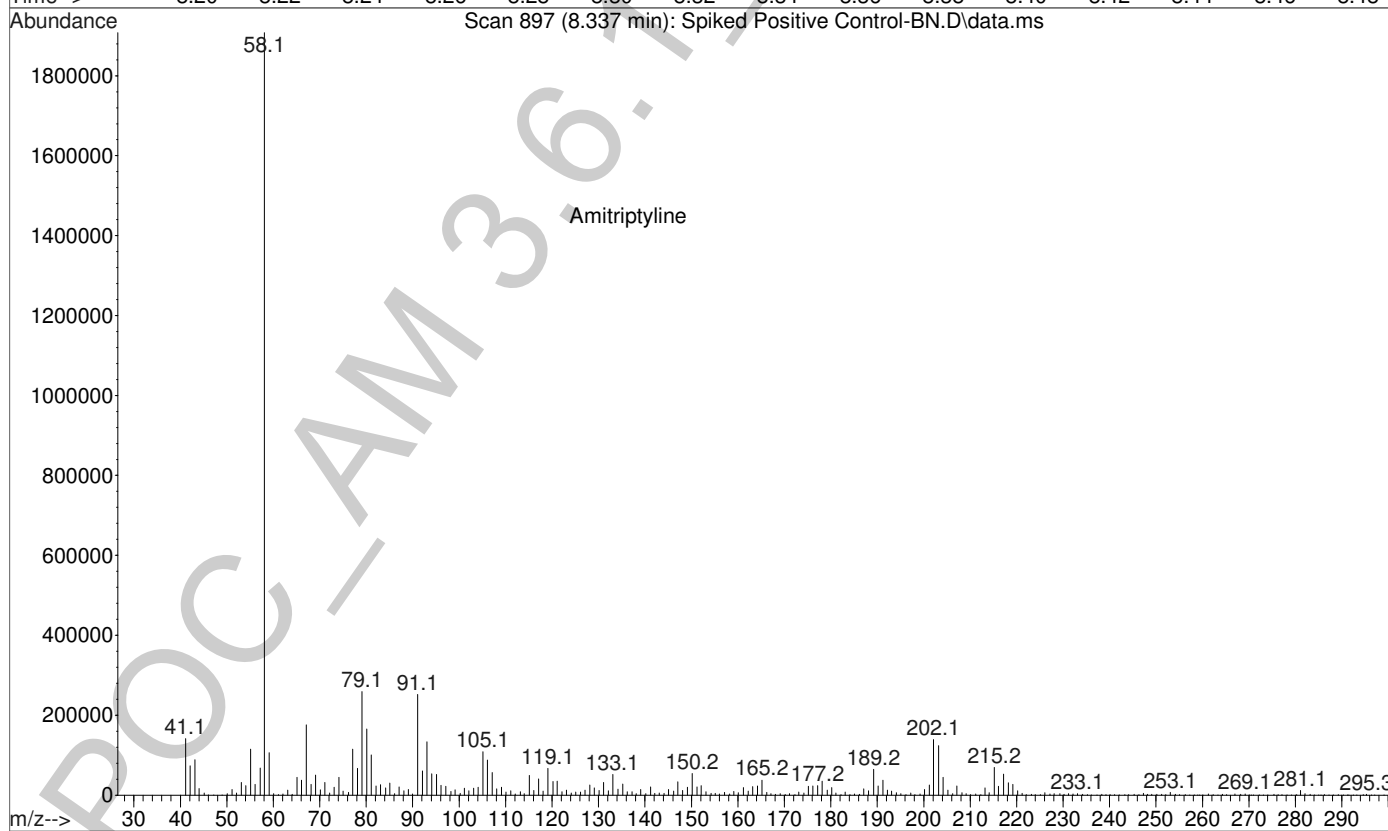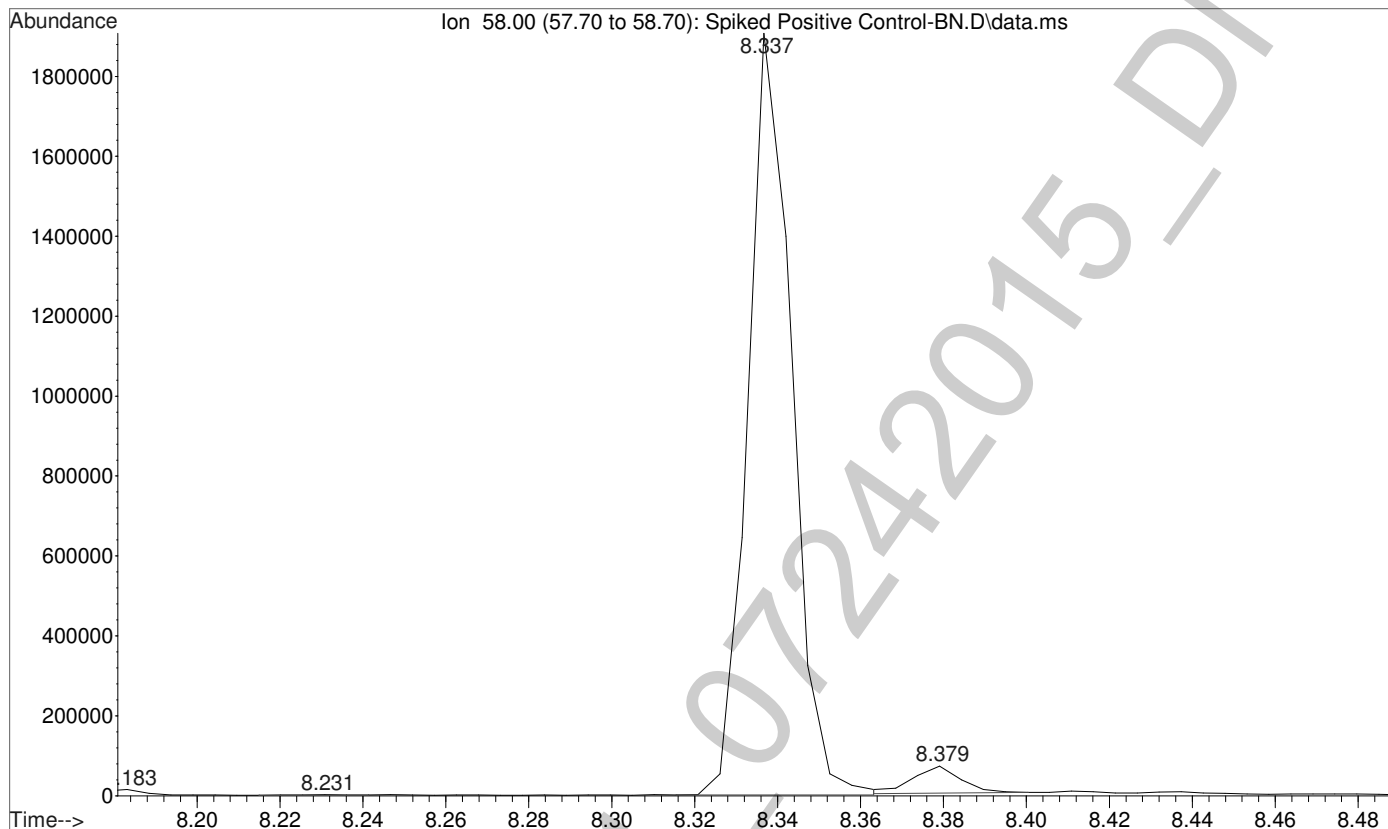



File :C:\gcms\1\data\Blood\072415\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 24 Jul 2015 12:27 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

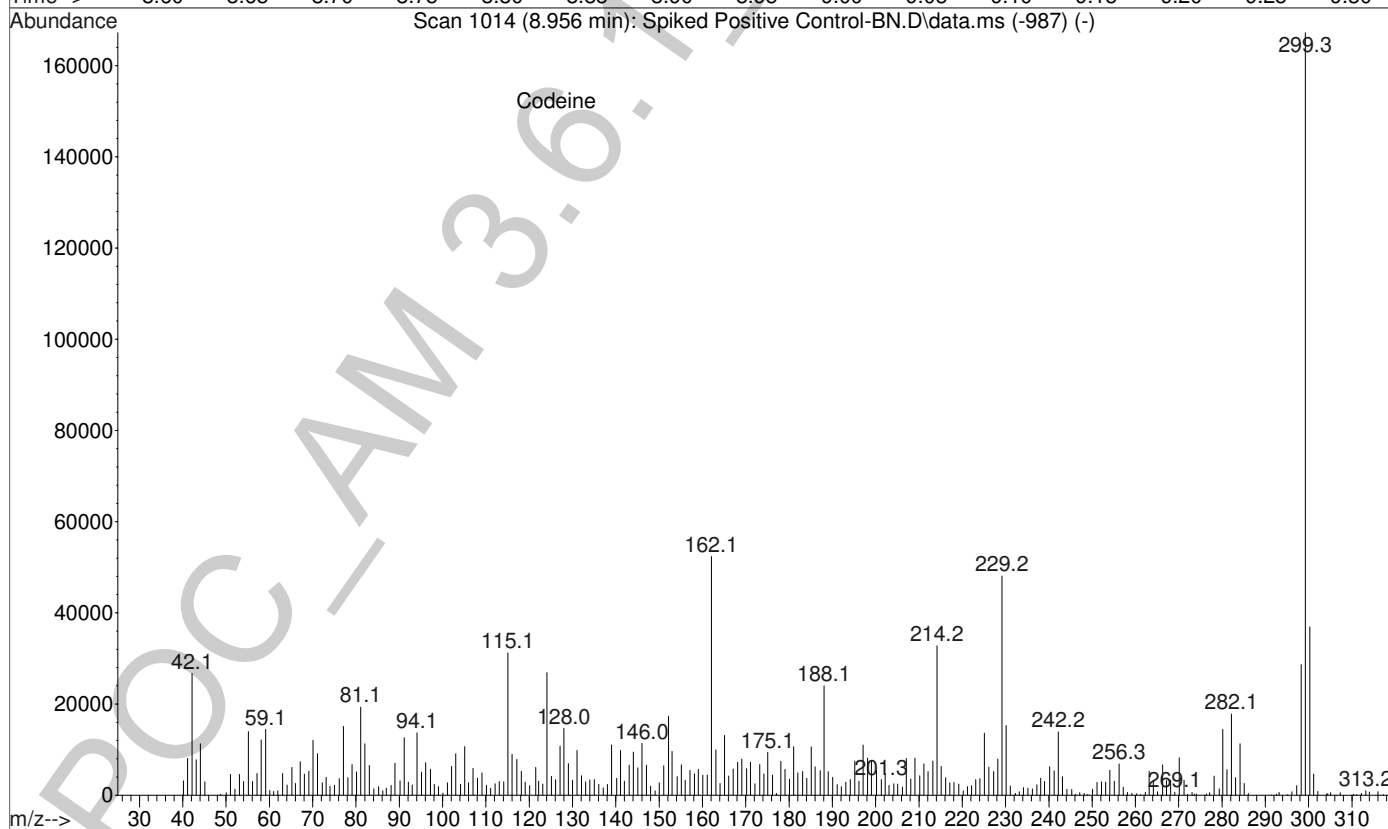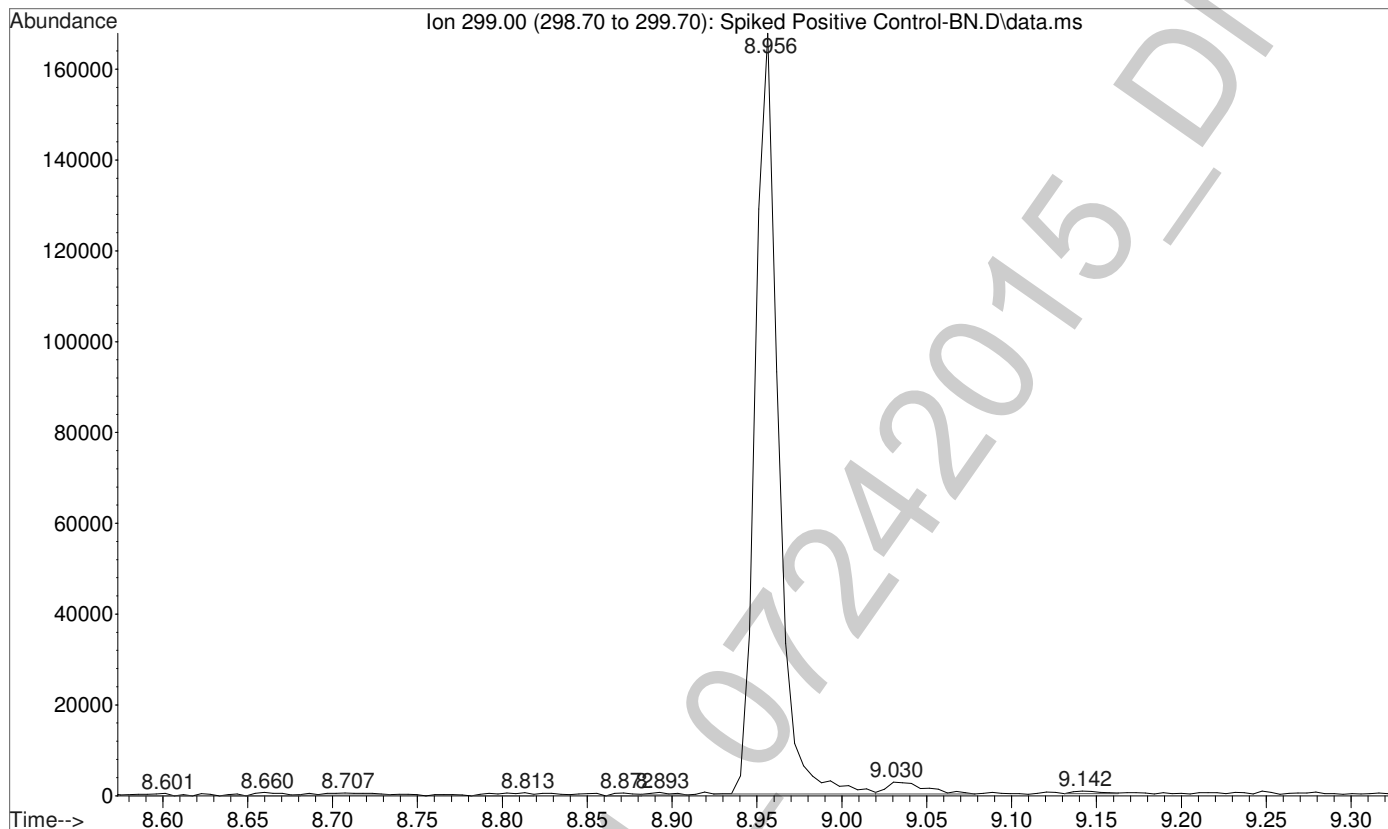


File :C:\gcms\1\data\Blood\072415\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 24 Jul 2015 12:27 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

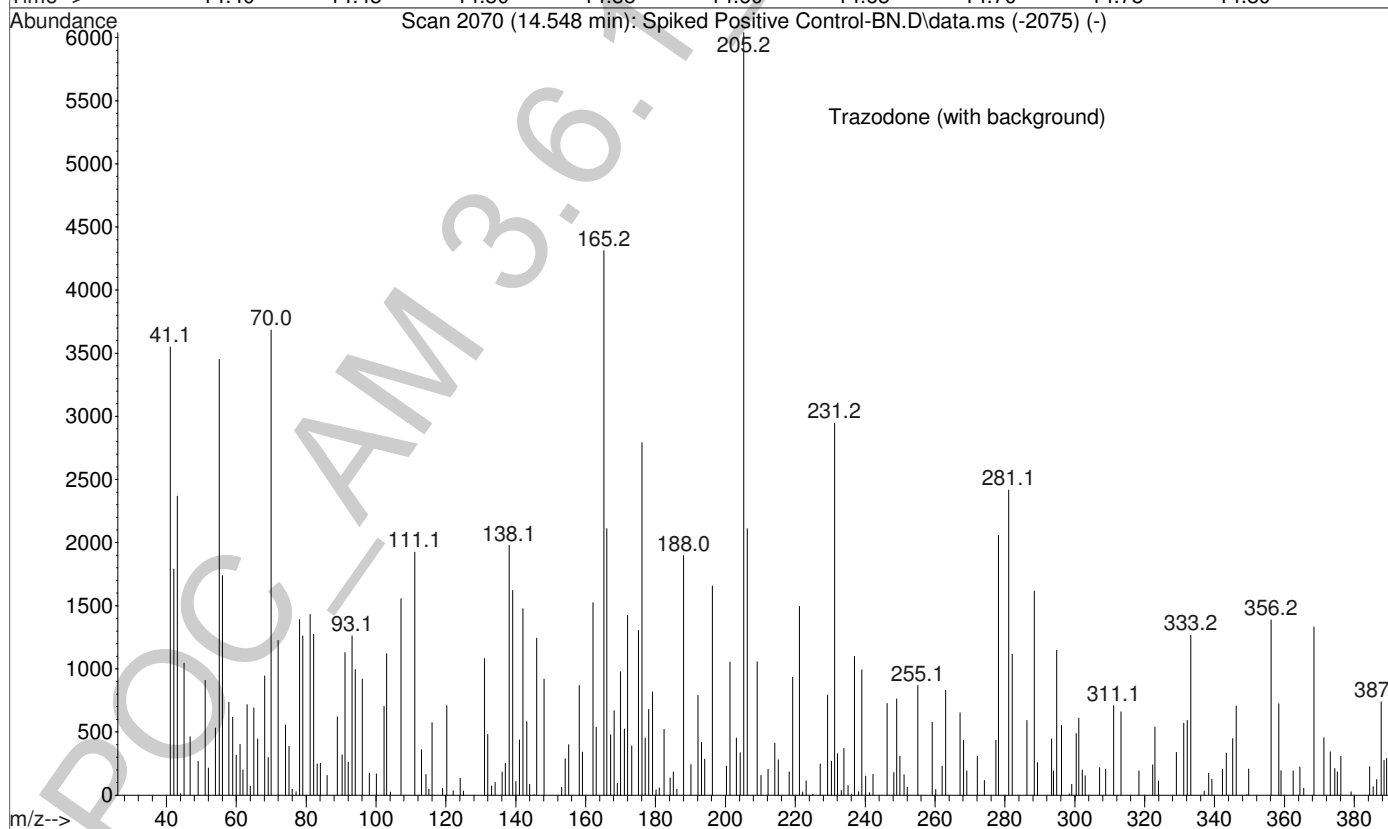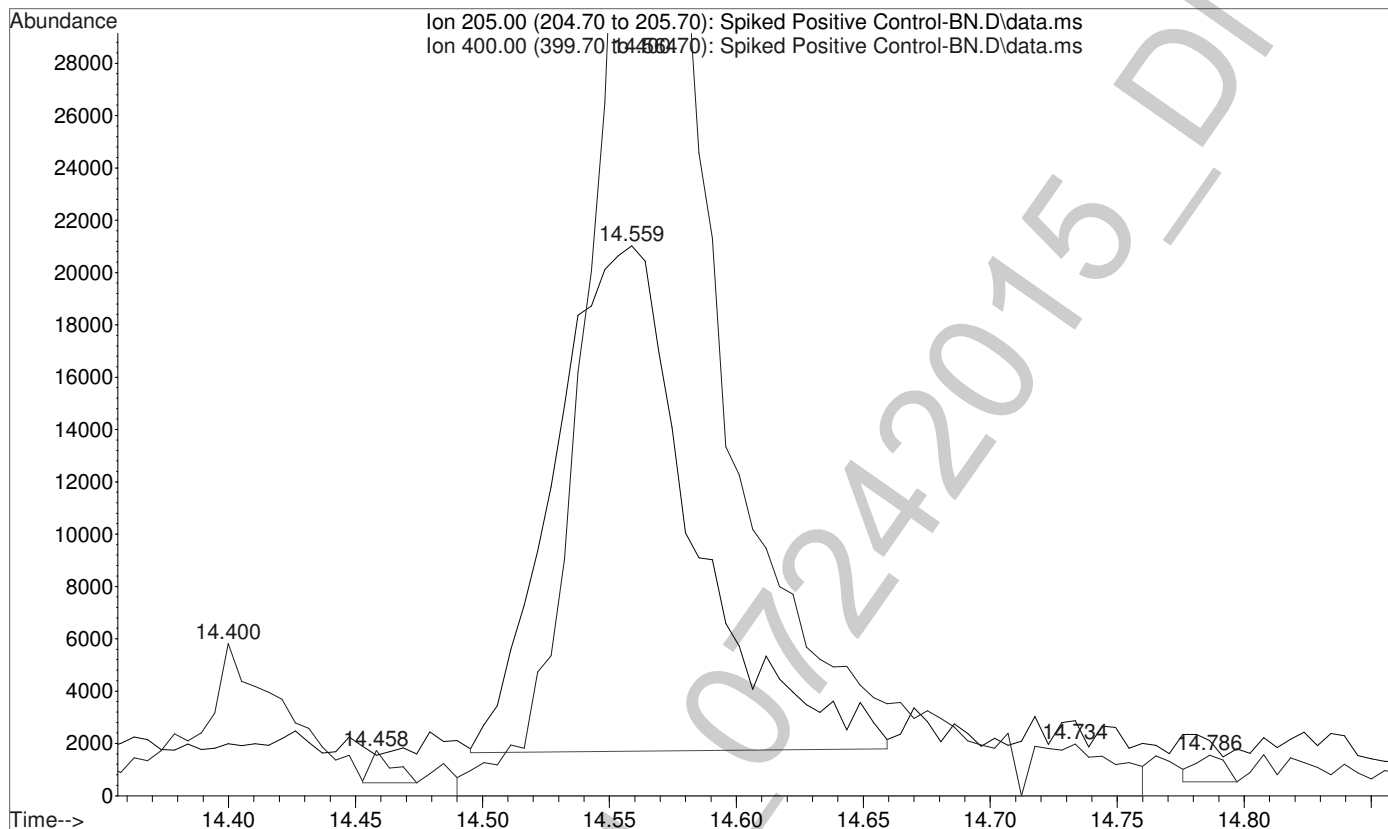

File :C:\gcms\1\data\Blood\072415\prbLK2.D
Operator : ISP\datastor
Acquired : 24 Jul 2015 12:50 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Solvent Blank
Misc Info : Chloroform
Vial Number: 99

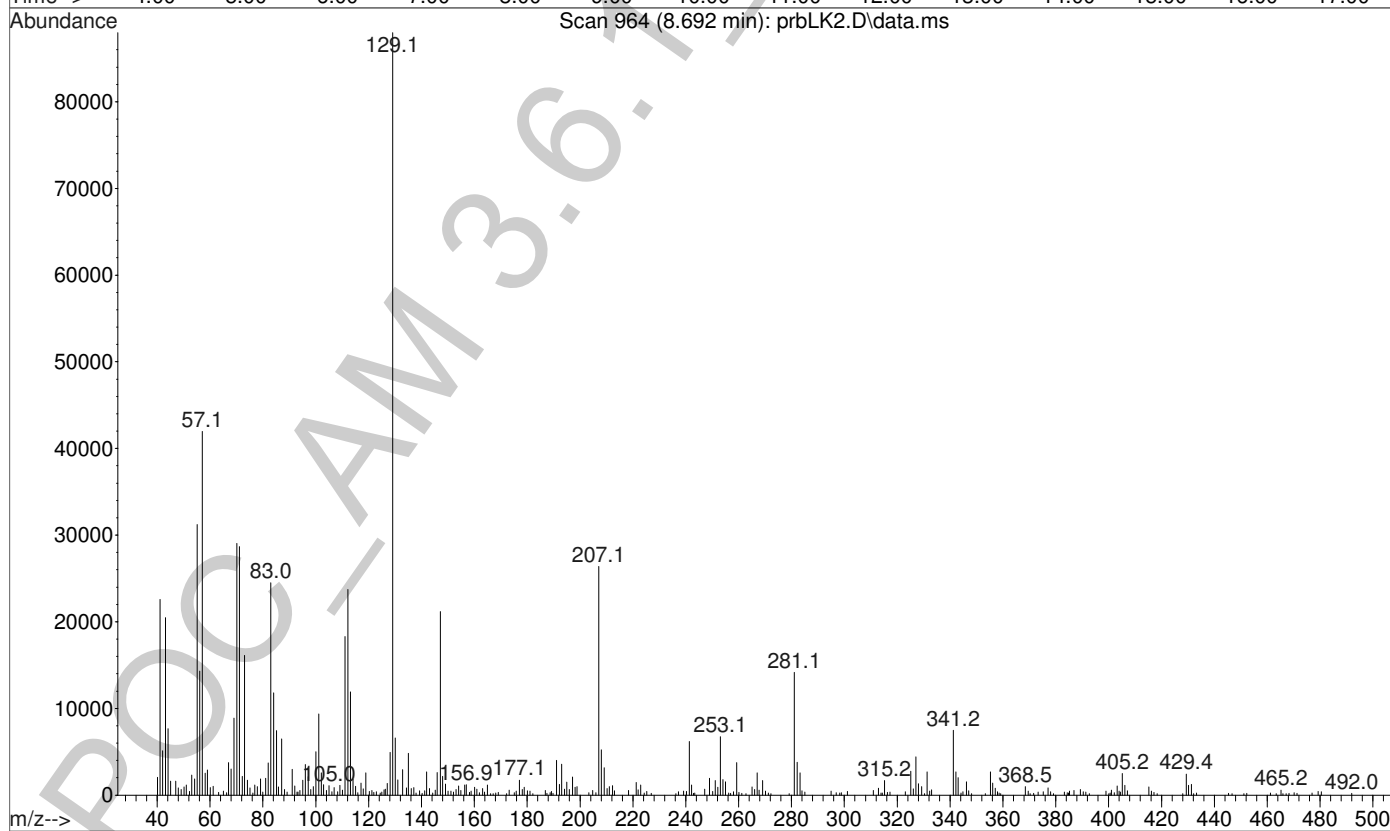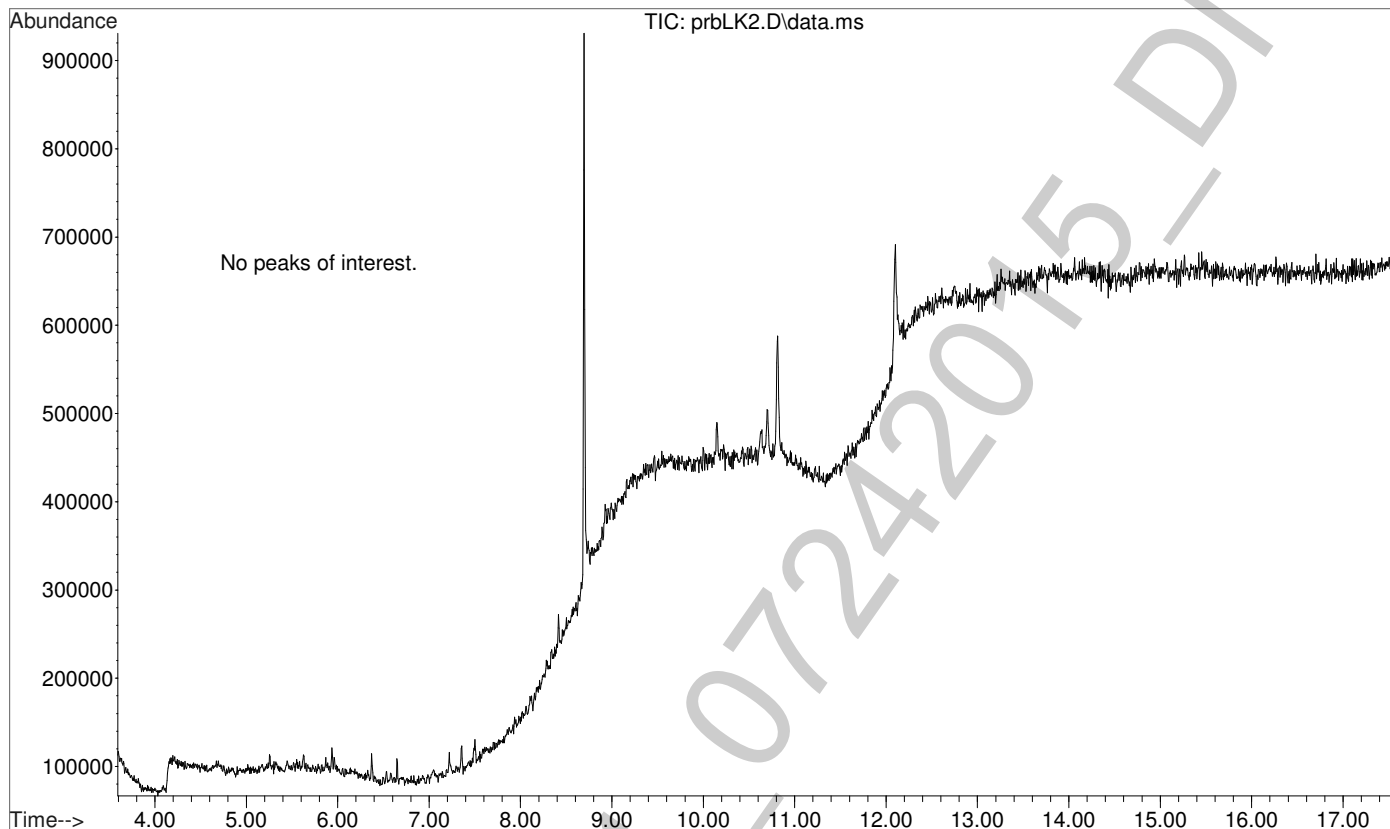



Analytical Method 3.6.1 & 3.6.7 QA Check List

Run Start Date: 07/24/15

Analyst: DND

(Long GC/MS temperature program)

Positive Control Compound List



- Methamphetamine
- Nicotine
- Meperidine
- Caffeine
- Diphenhydramine
- Lidocaine
- PCP
- Methadone
- Amitriptyline
- Codeine
- Trazodone

Internal Standards


- Benzphetamine
- Papaverine

Optional back extraction **not** performed.
Samples reconstituted in methanol.



File :C:\gcms\1\data\Blood\072415\Reinjection Longer GC Method\Pre
... run Solvent Blankr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 24 Jul 2015 13:13 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Pre-run Solvent Blank
Misc Info : Chloroform

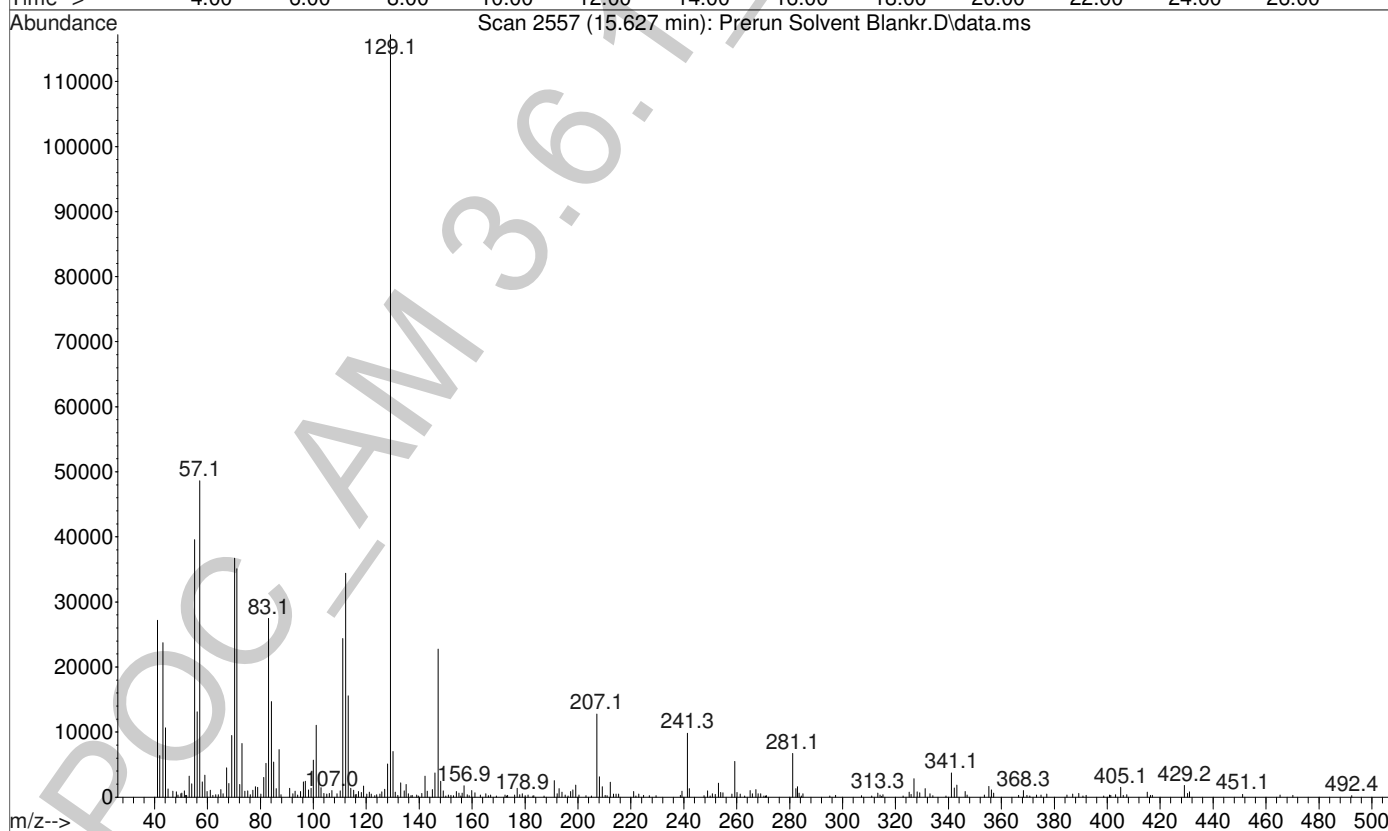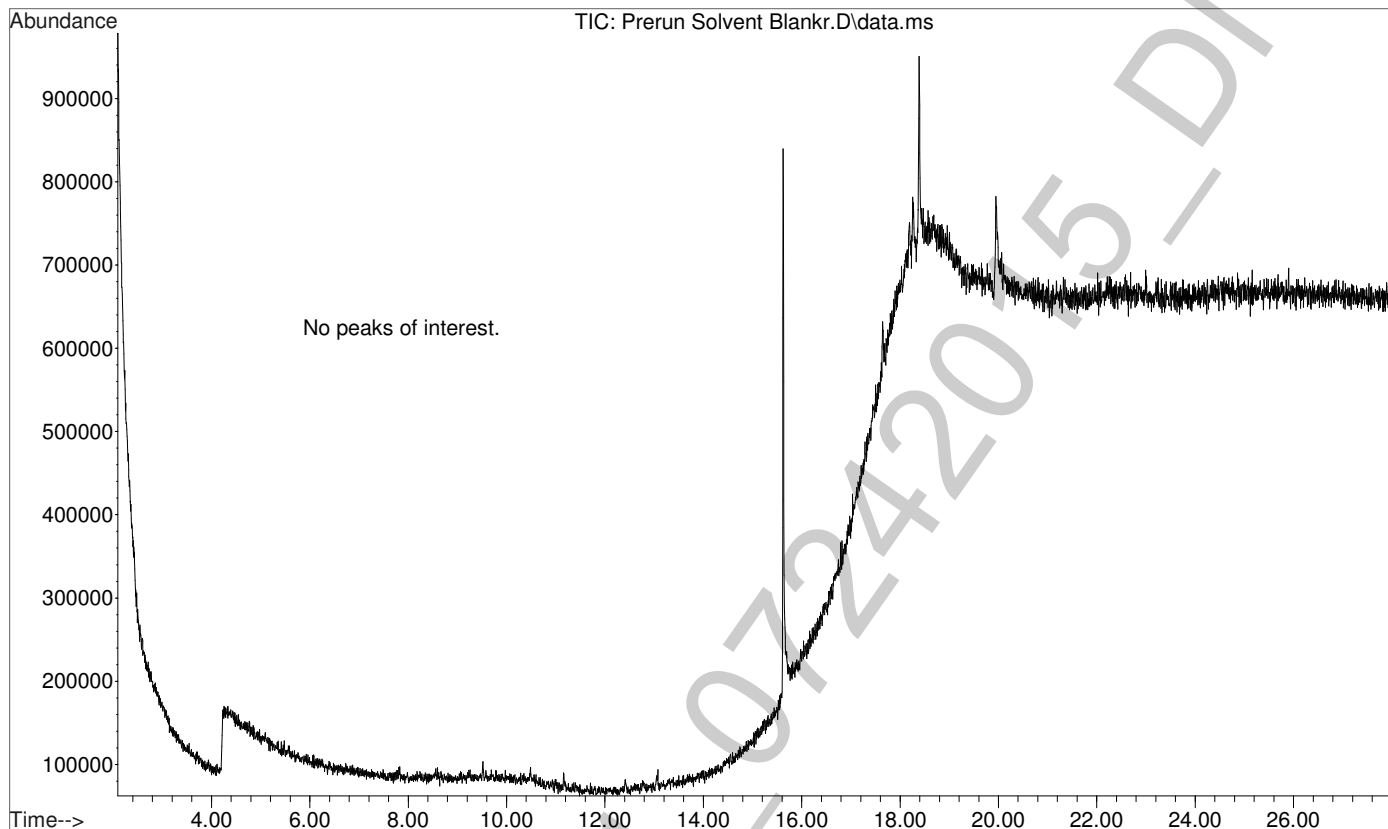



File :C:\gcms\1\data\Blood\072415\Reinjection Longer GC Method\Neg
... ative Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 24 Jul 2015 13:47 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1

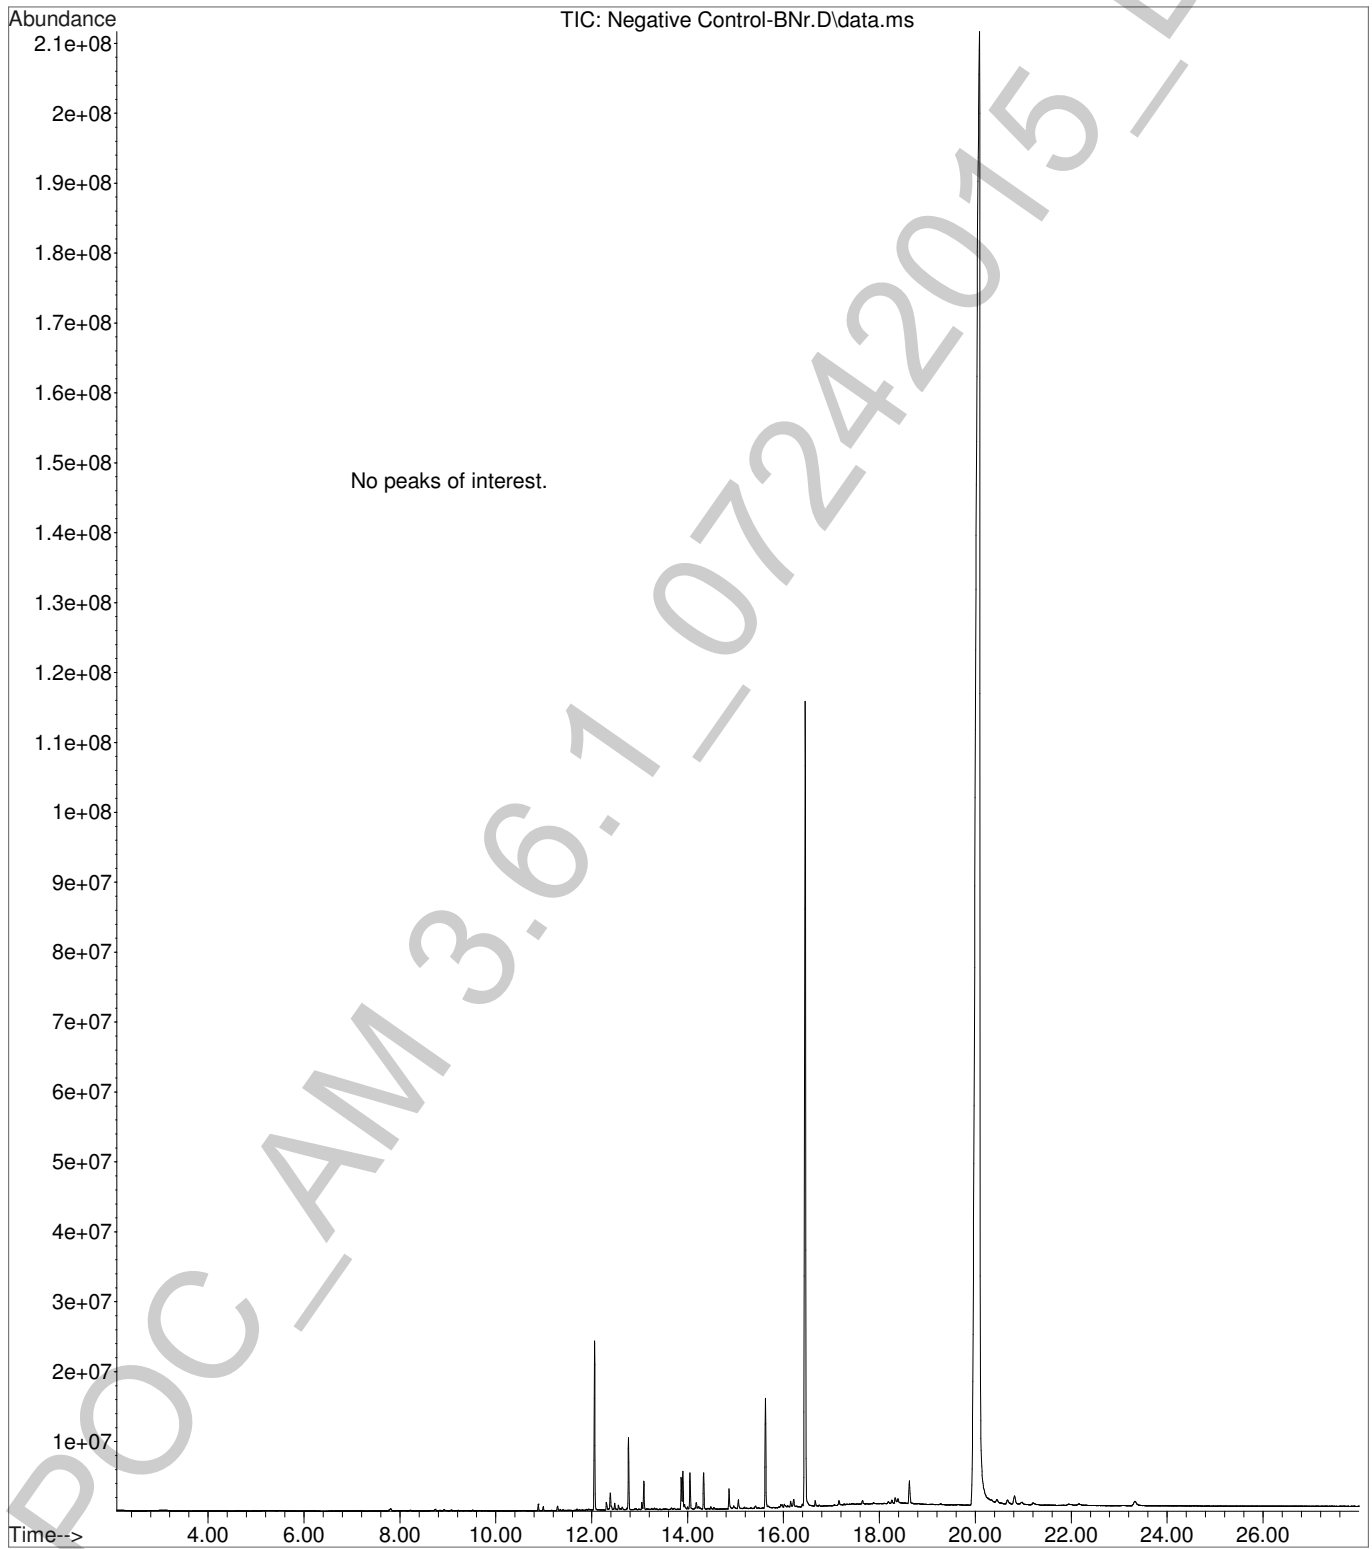

File :C:\gcms\1\data\Blood\072415\Reinjection Longer GC Method\Neg
... ative Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 24 Jul 2015 13:47 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1

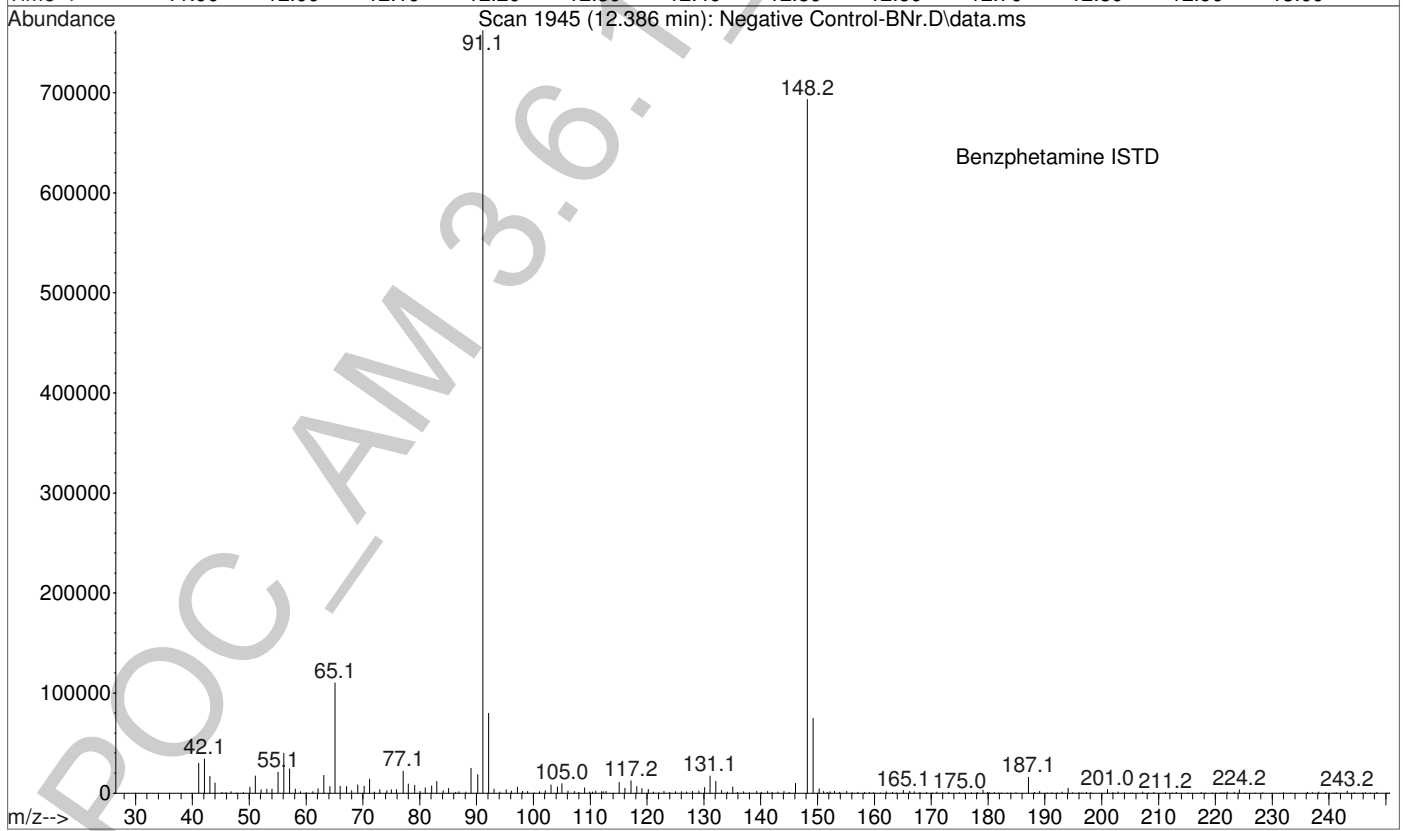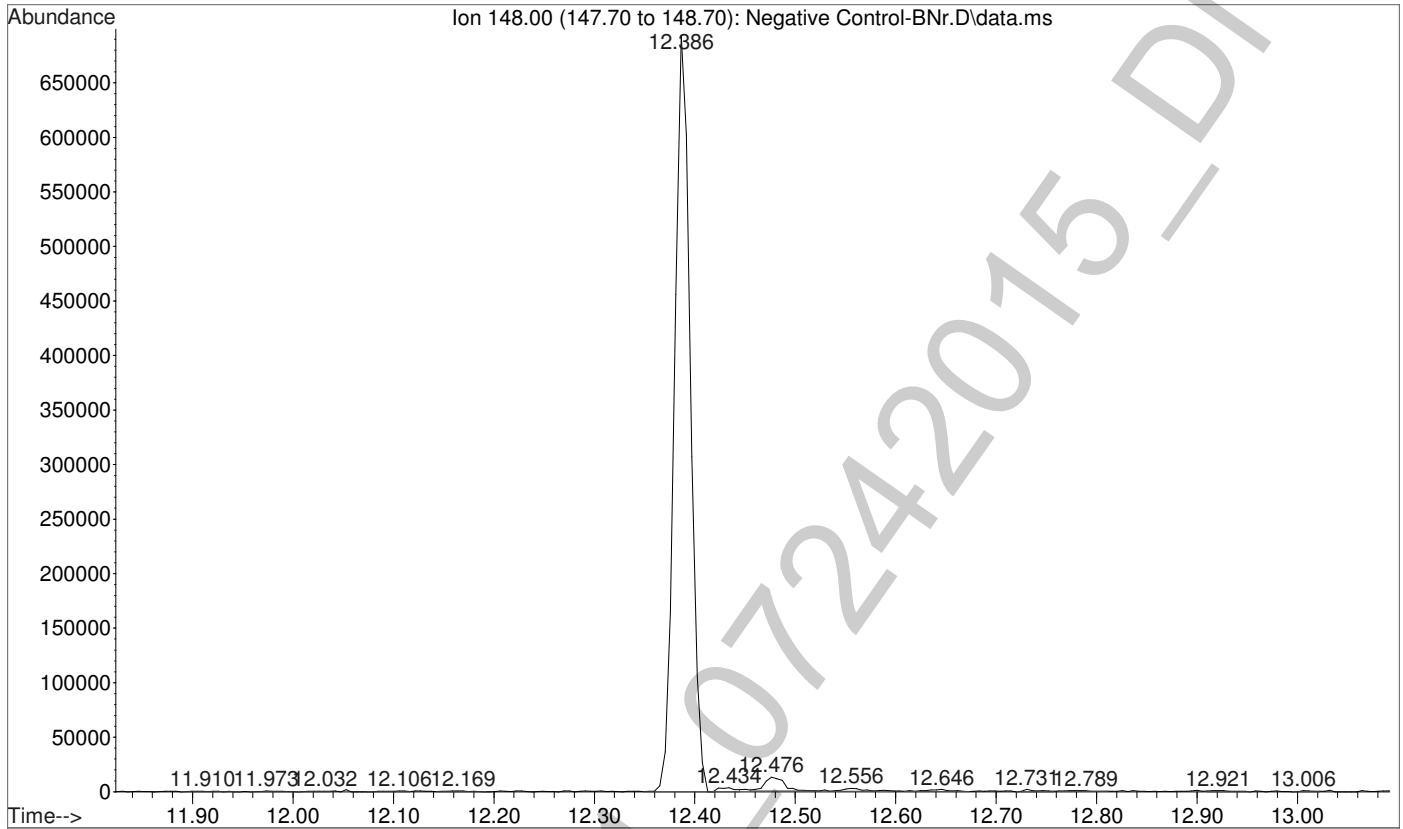


File :C:\gcms\1\data\Blood\072415\Reinjection Longer GC Method\Neg
... ative Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 24 Jul 2015 13:47 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1

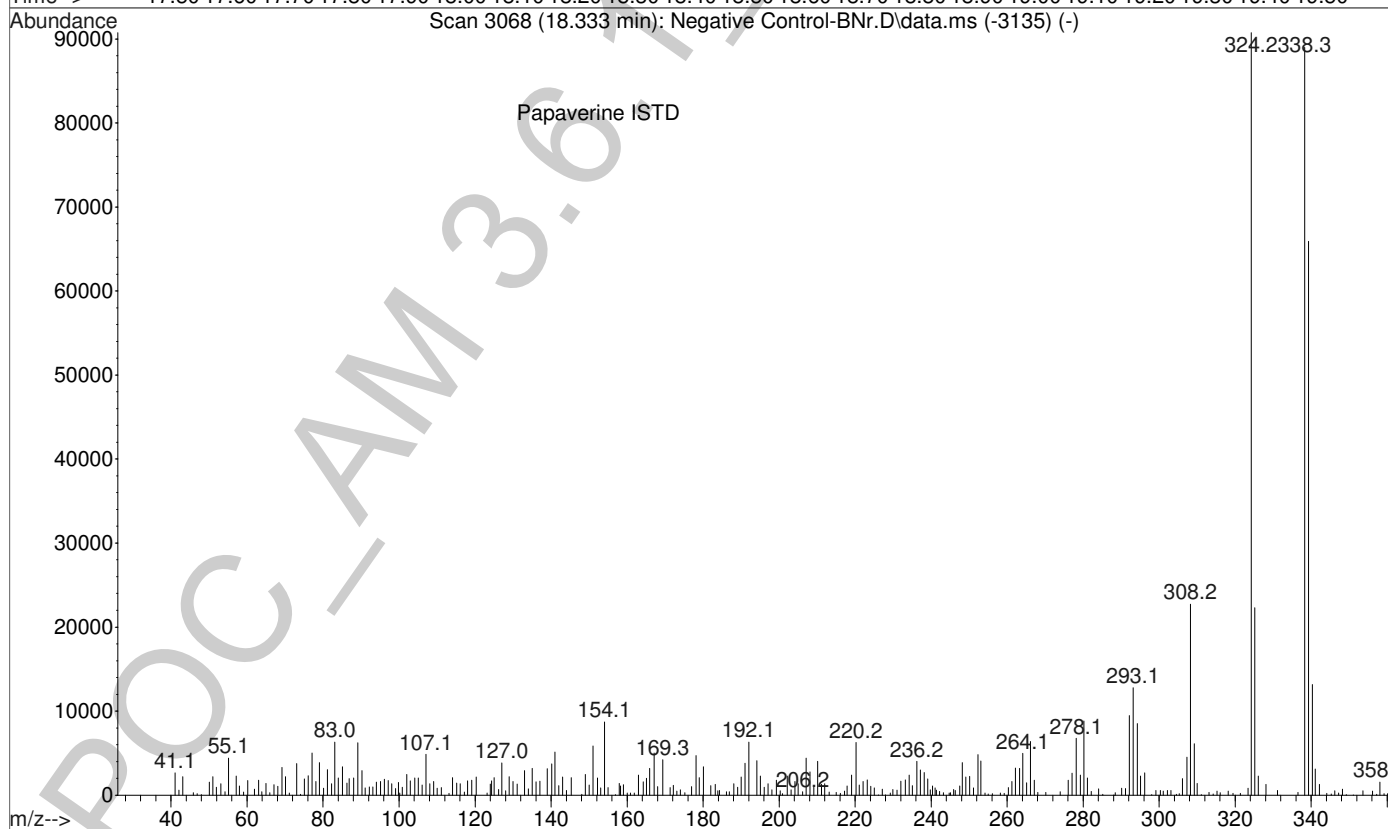
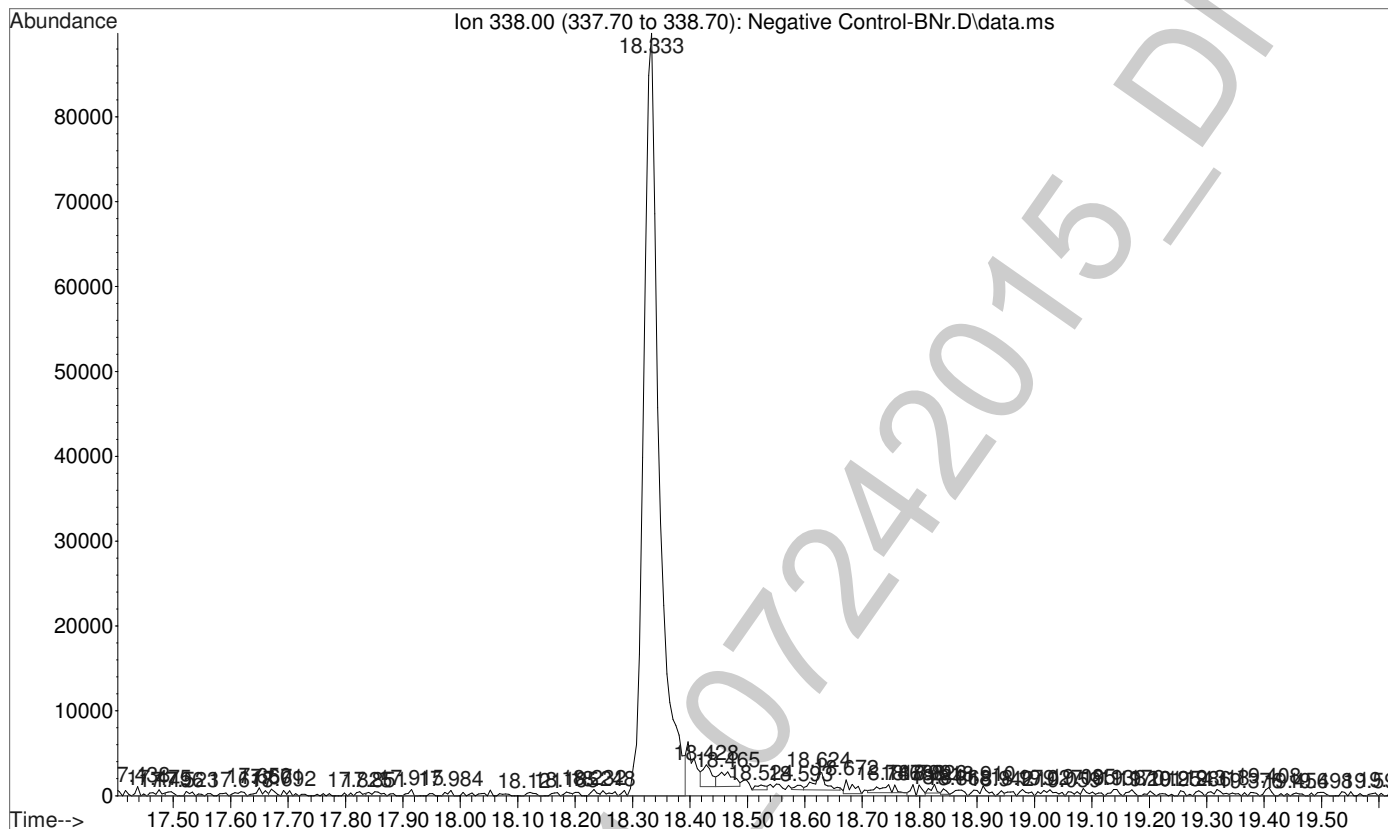






File :C:\gcms\1\data\Blood\072415\Reinjection Longer GC Method\Spi
... ked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 24 Jul 2015 14:21 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

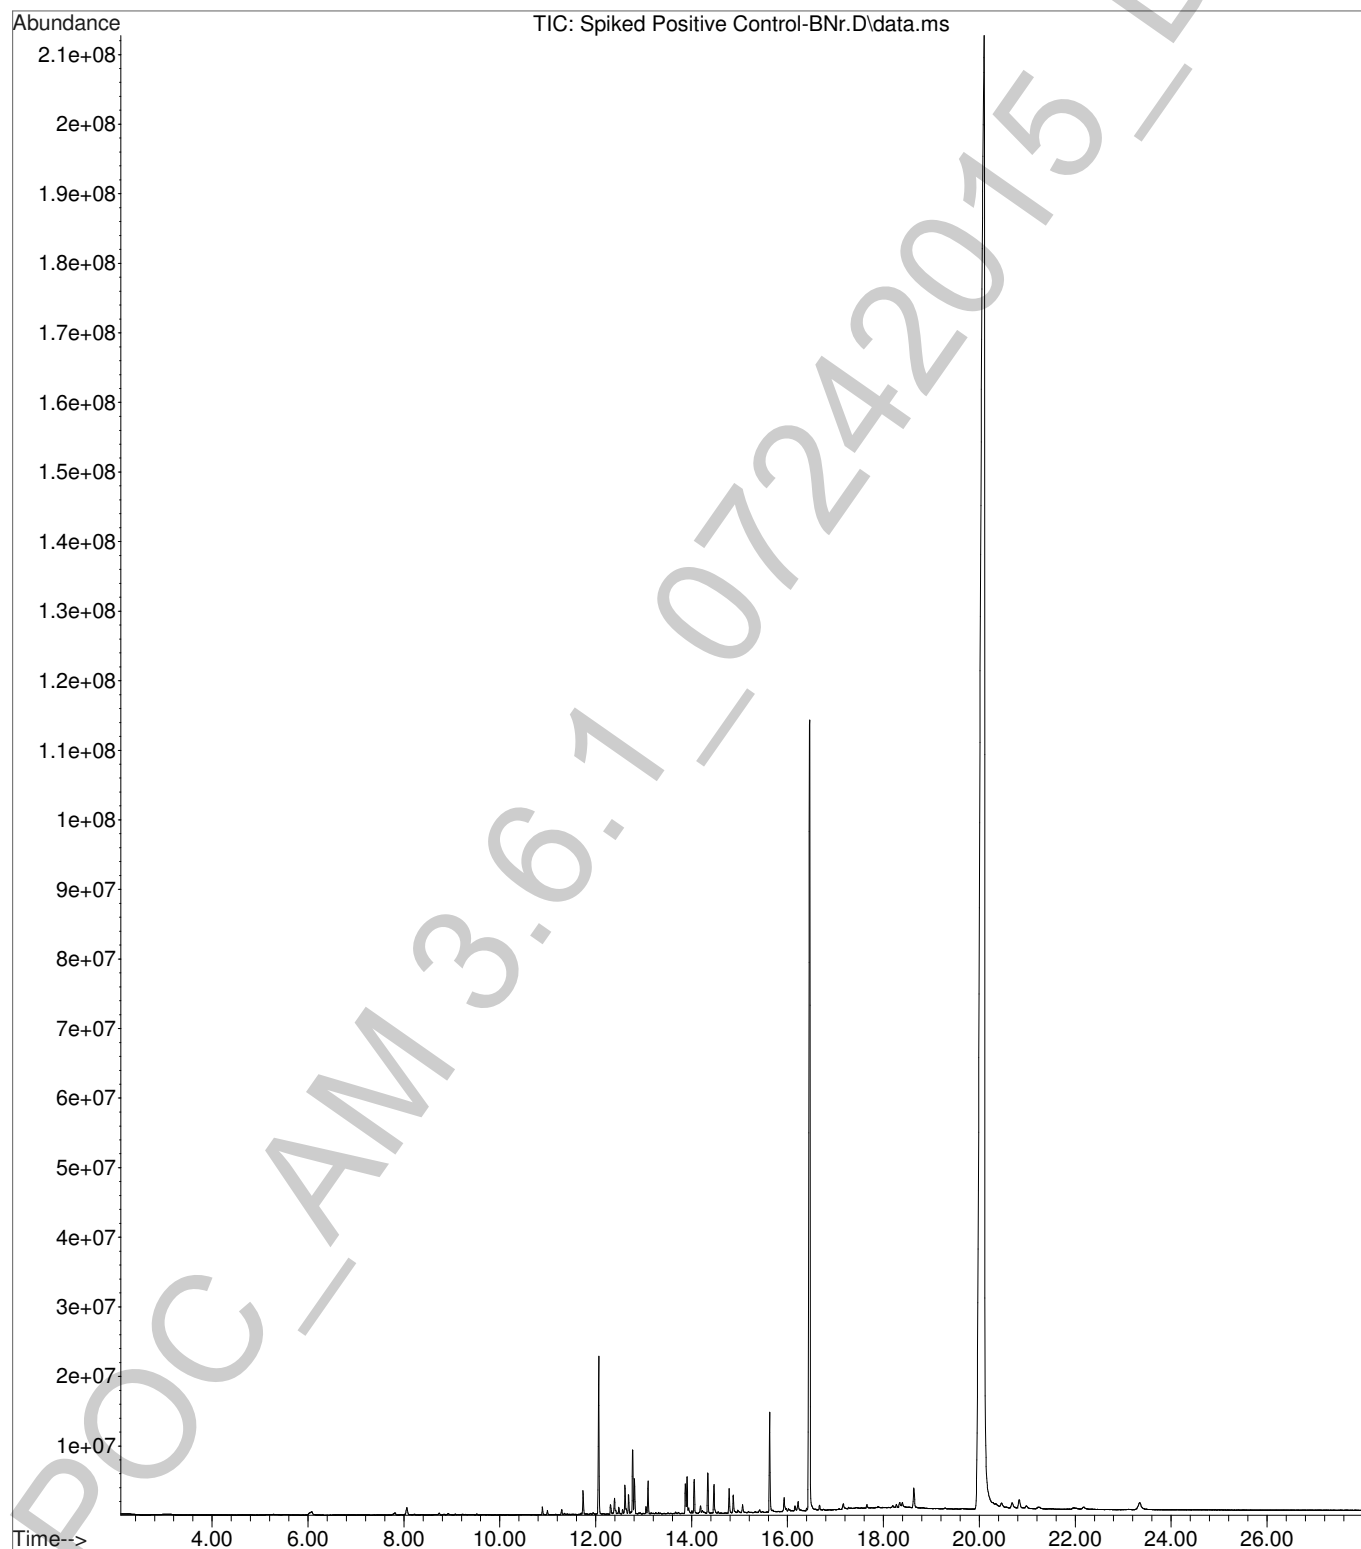

File :C:\gcms\1\data\Blood\072415\Reinjection Longer GC Method\Spi
... ked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 24 Jul 2015 14:21 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

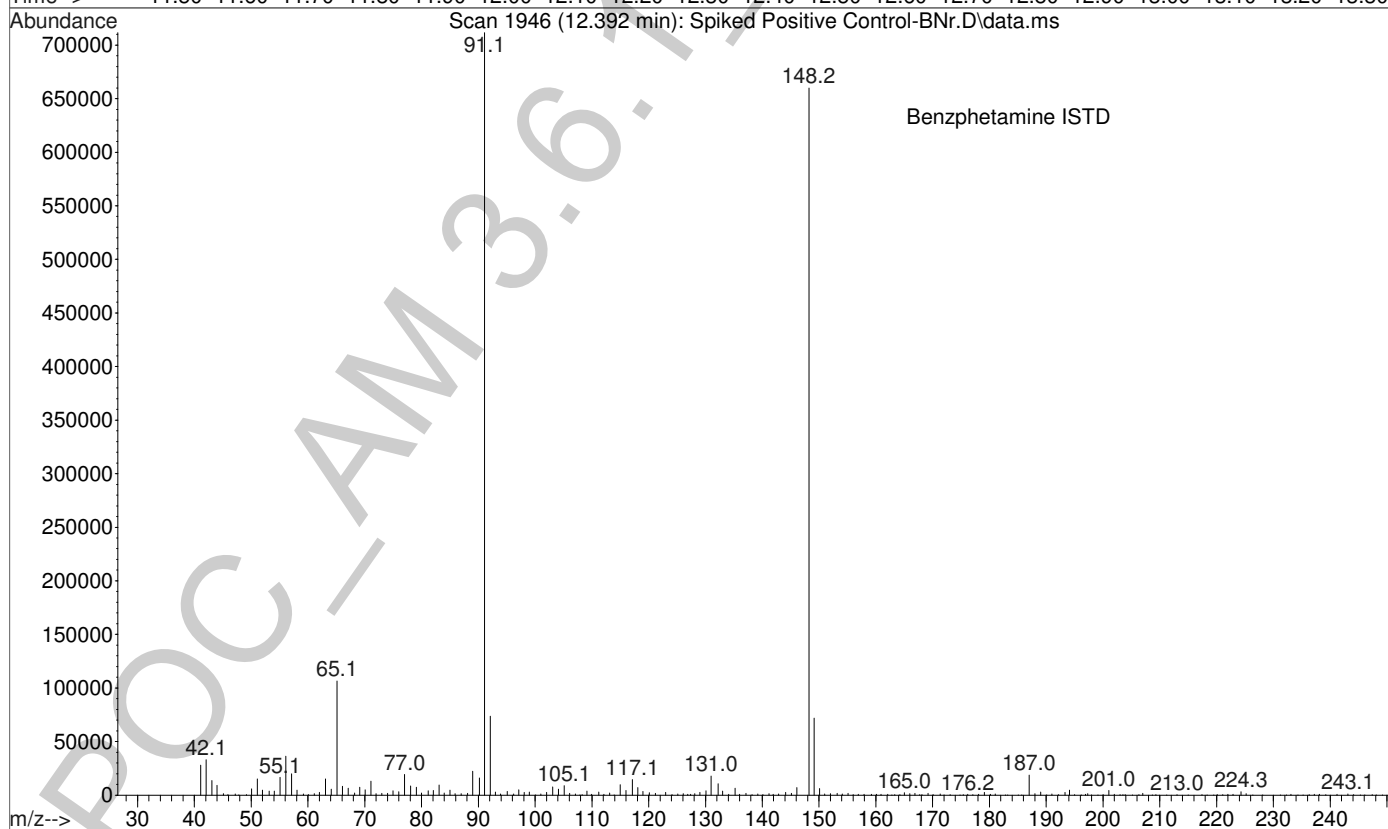
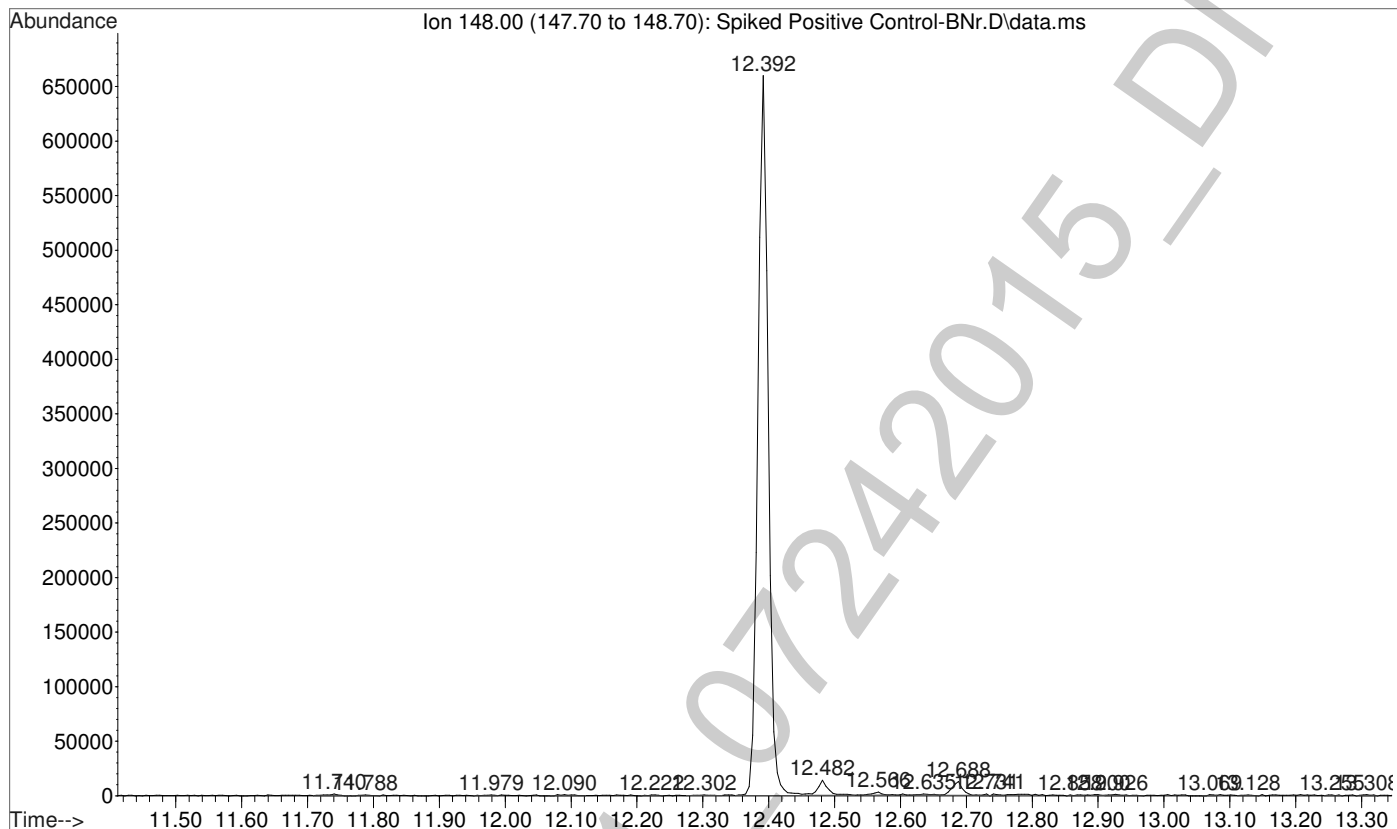


File :C:\gcms\1\data\Blood\072415\Reinjection Longer GC Method\Spi
... ked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 24 Jul 2015 14:21 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

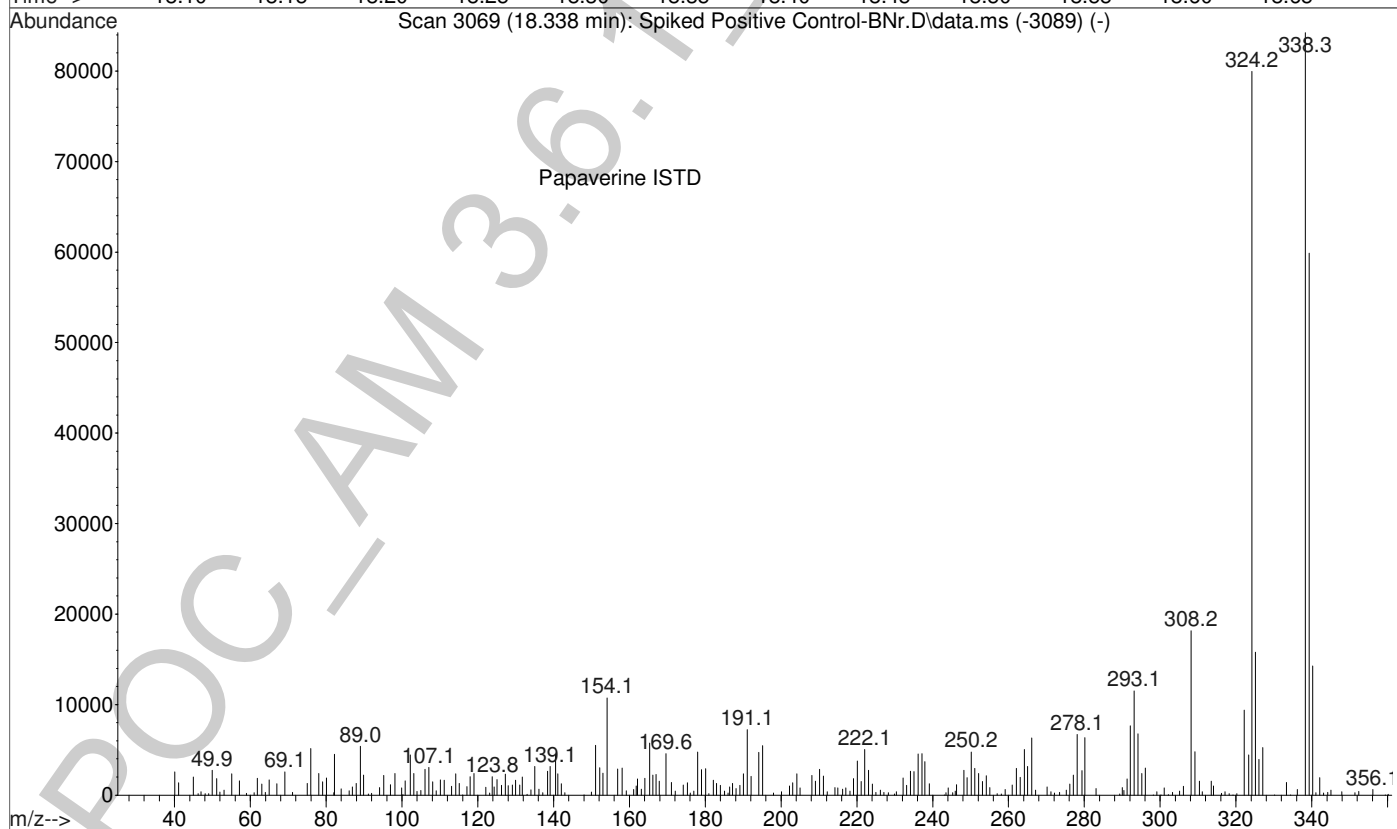
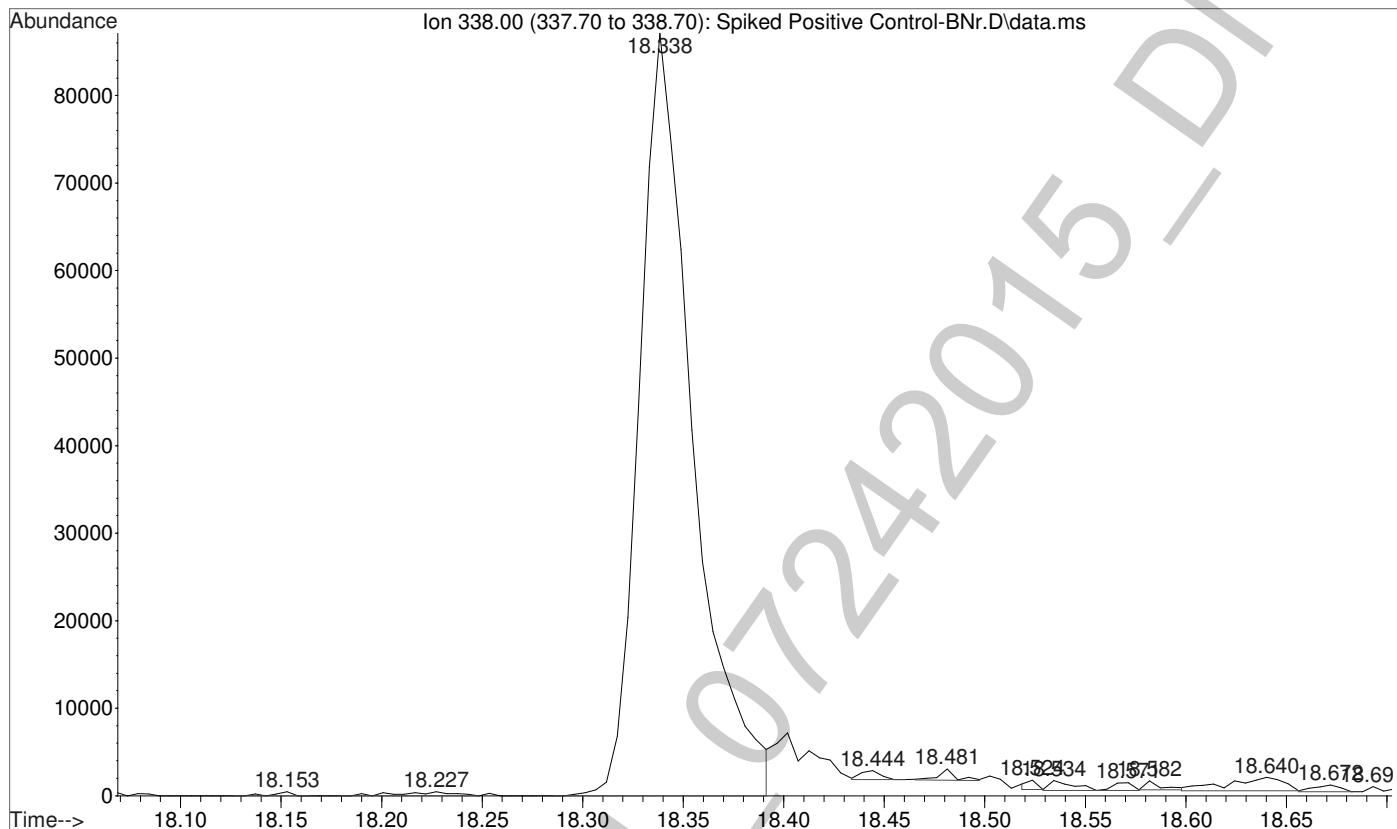






File :C:\gcms\1\data\Blood\072415\Reinjection Longer GC Method\Spiked Positive Control-BNr.D
...
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 24 Jul 2015 14:21 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

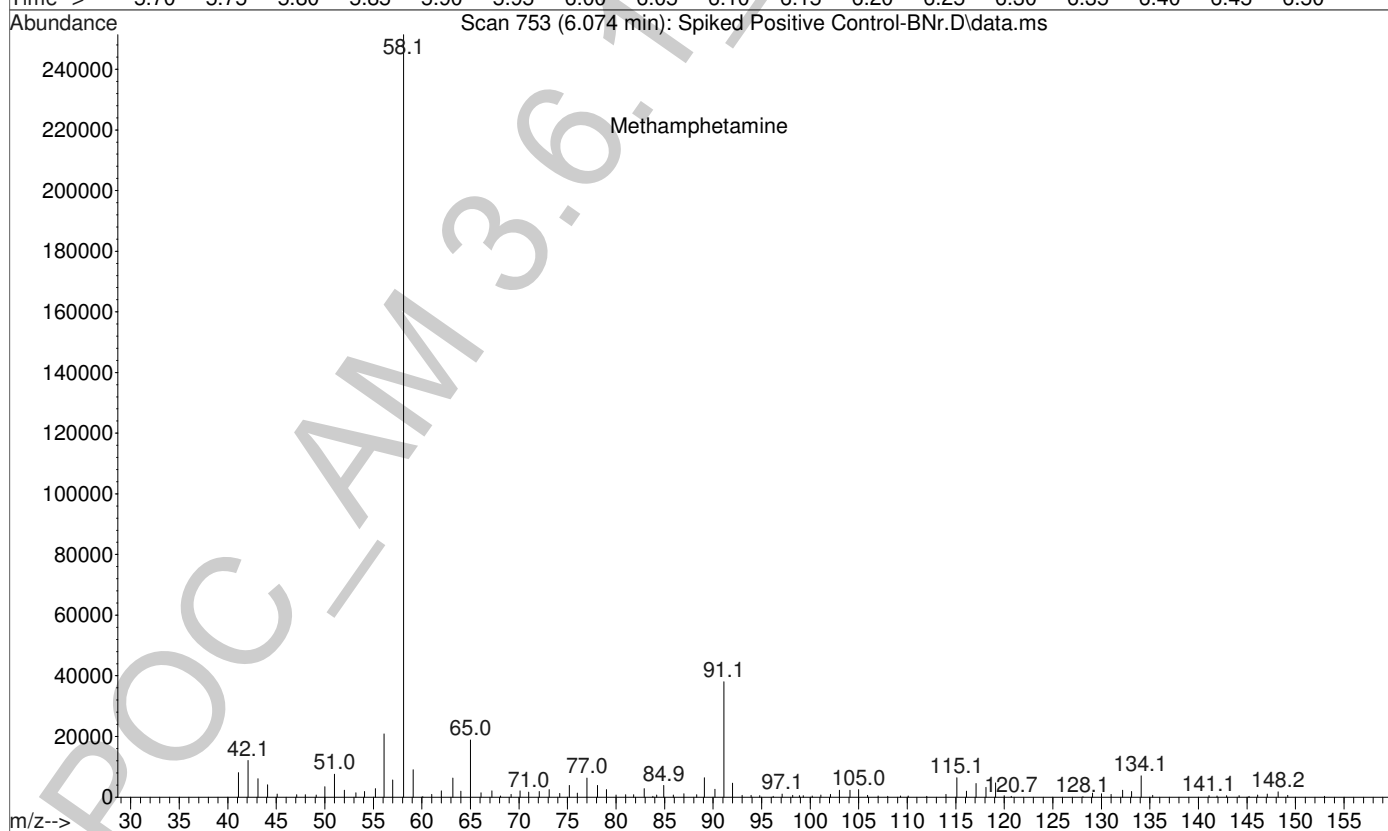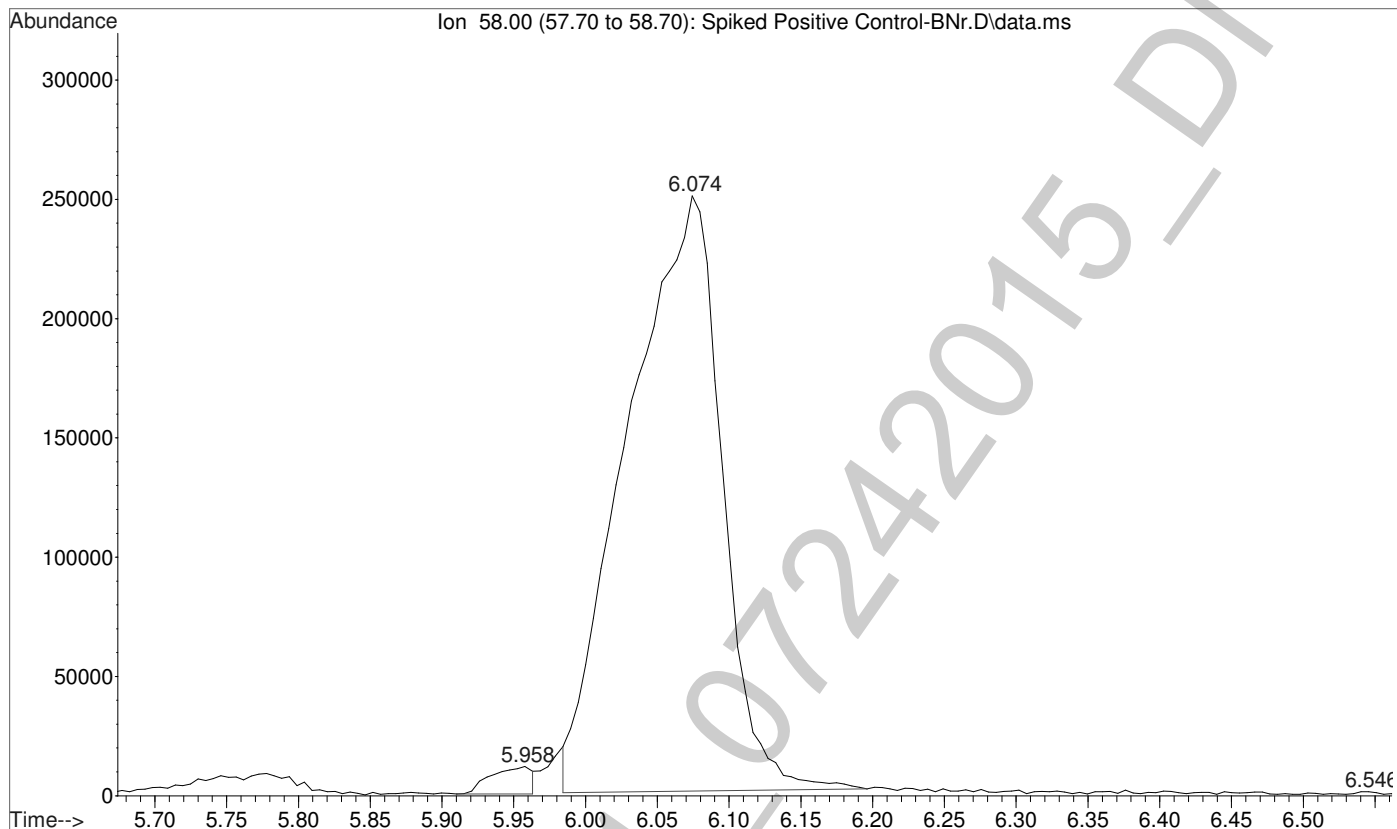



File :C:\gcms\1\data\Blood\072415\Reinjection Longer GC Method\Spiked Positive Control-BNr.D
...
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 24 Jul 2015 14:21 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

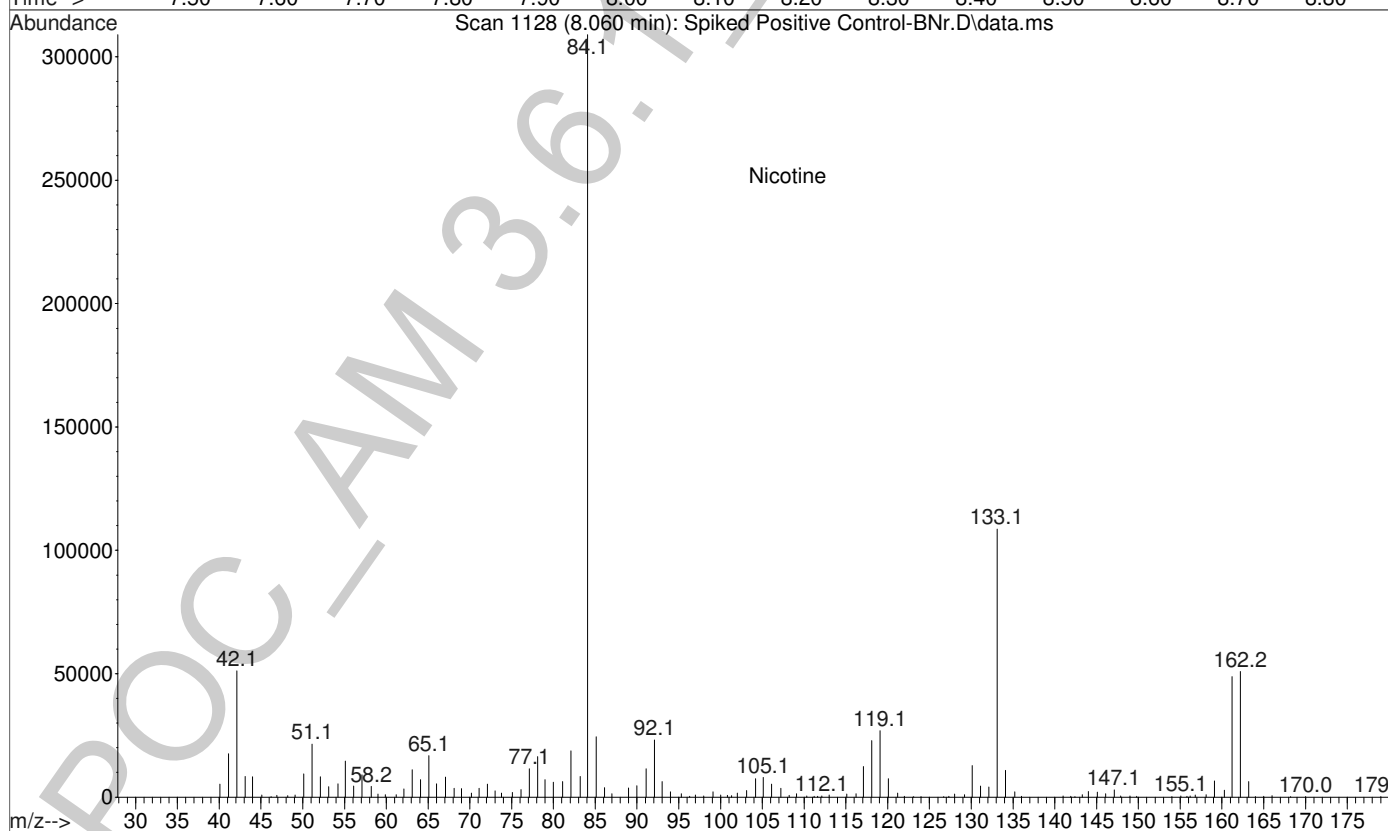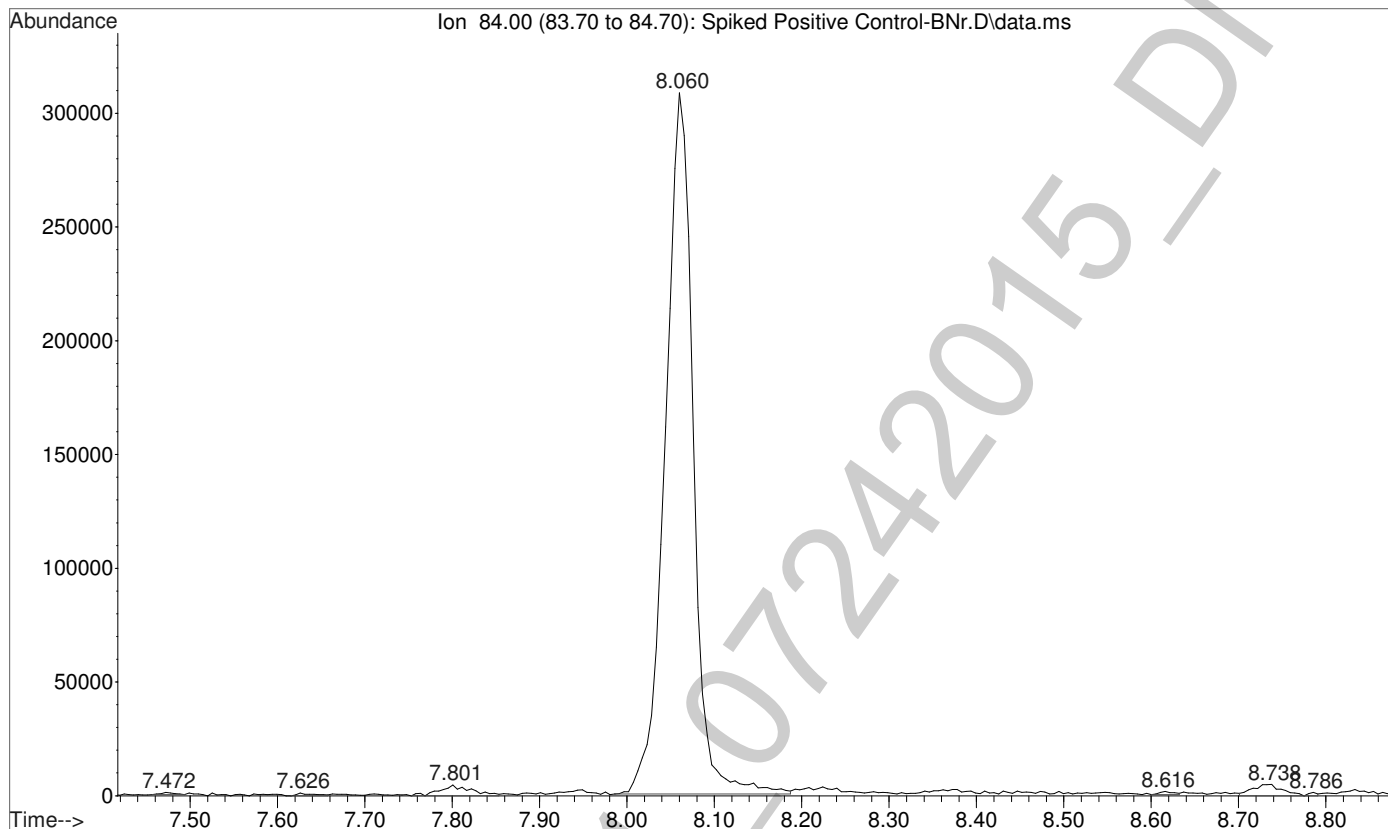



File :C:\gcms\1\data\Blood\072415\Reinjection Longer GC Method\Spiked Positive Control-BNr.D
...
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 24 Jul 2015 14:21 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

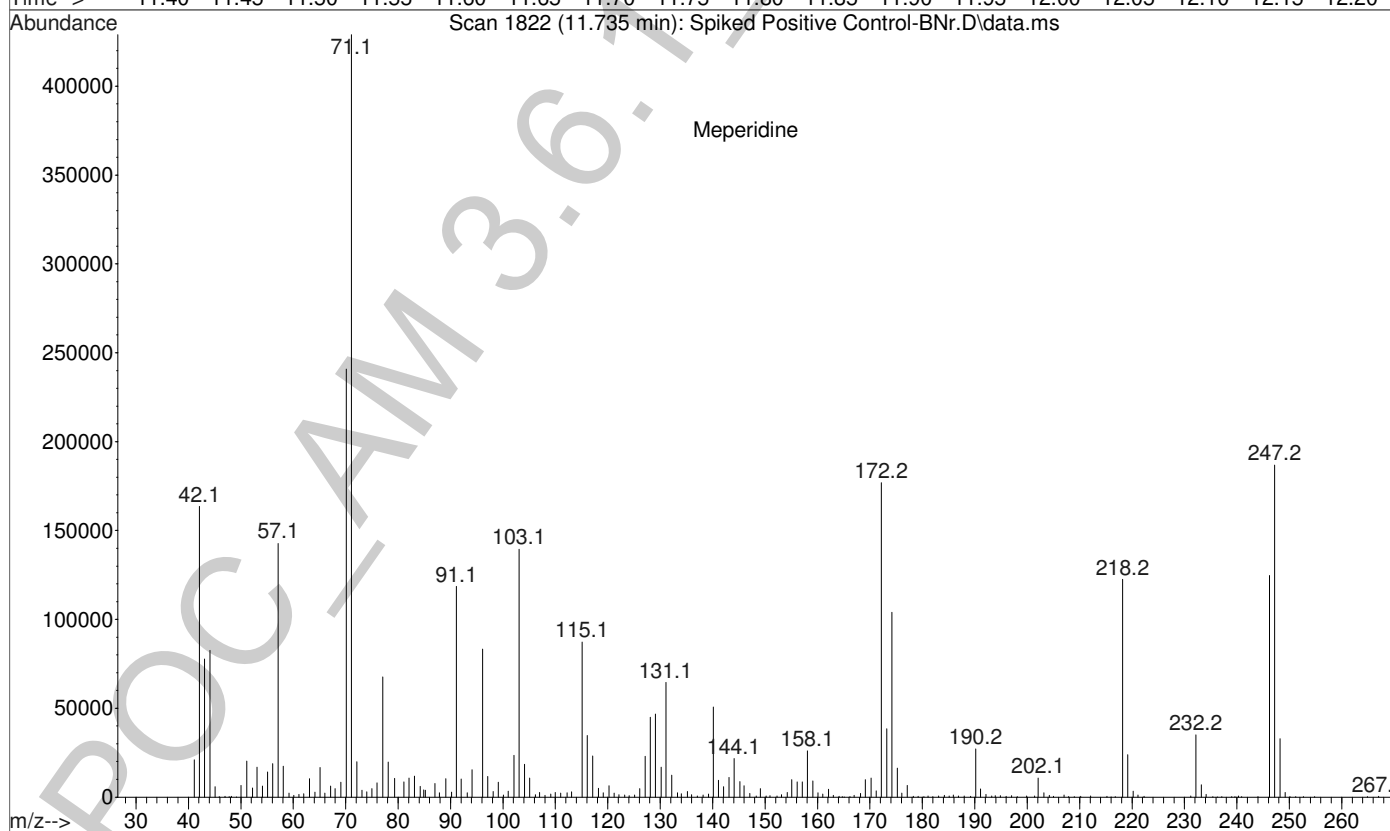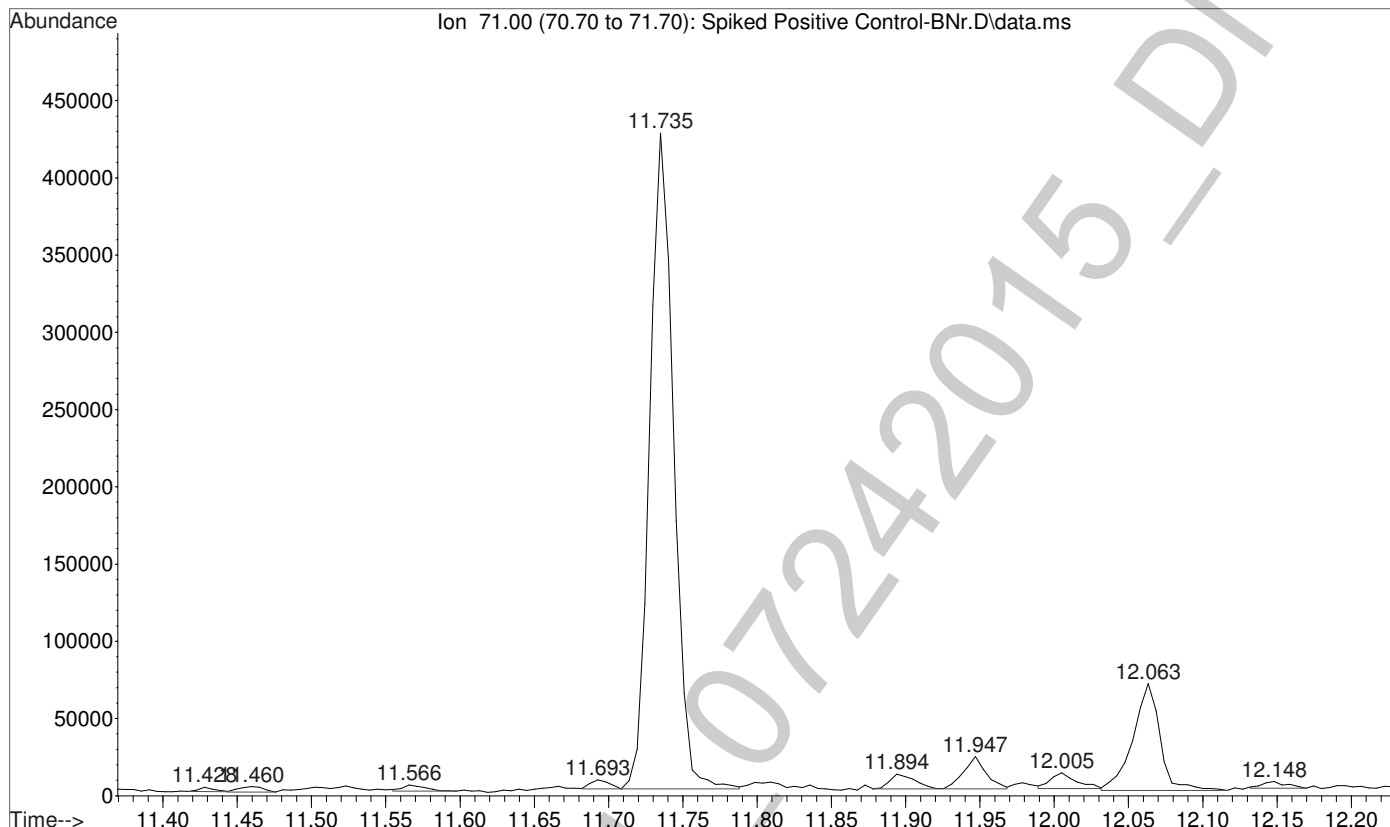



File :C:\gcms\1\data\Blood\072415\Reinjection Longer GC Method\Spiked Positive Control-BNr.D
...
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 24 Jul 2015 14:21 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

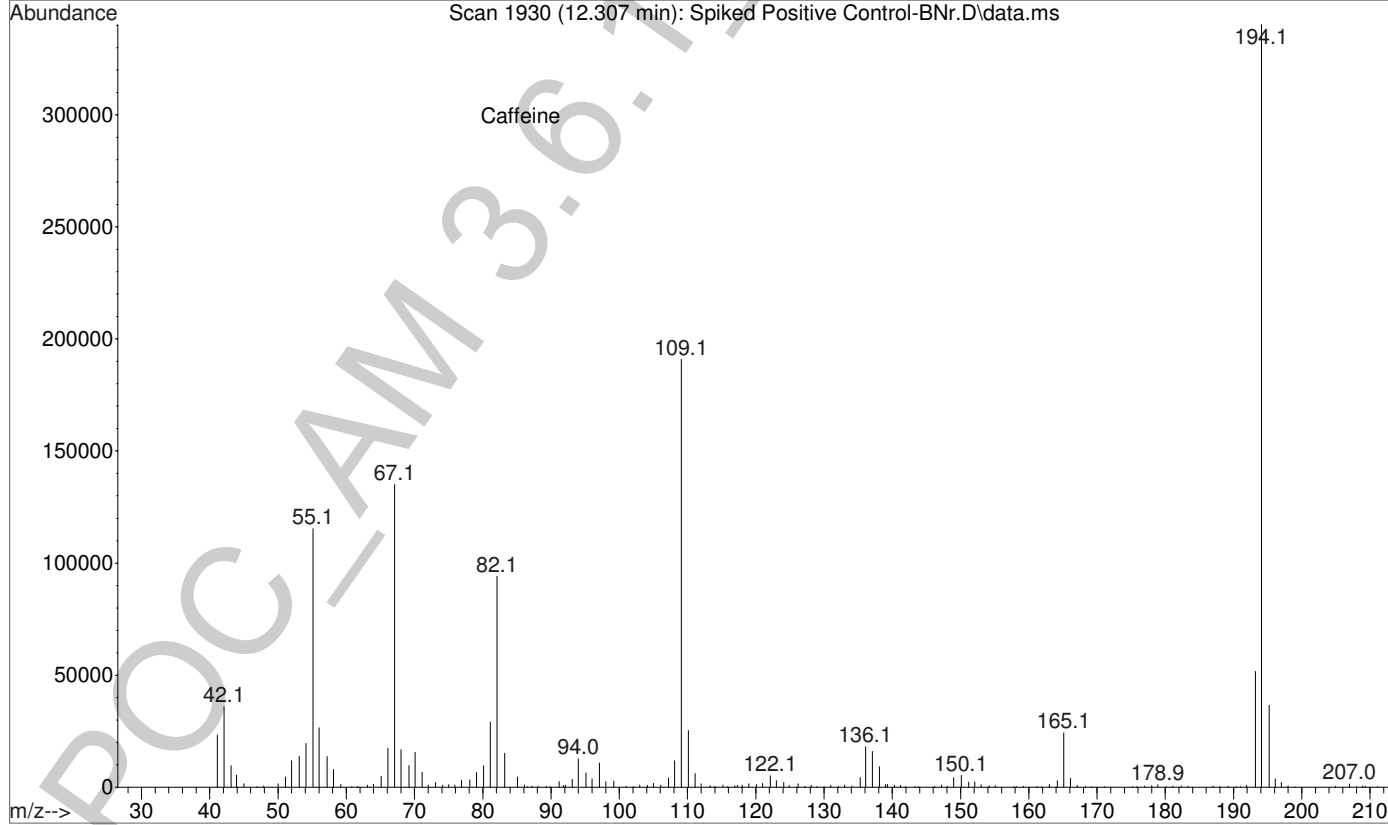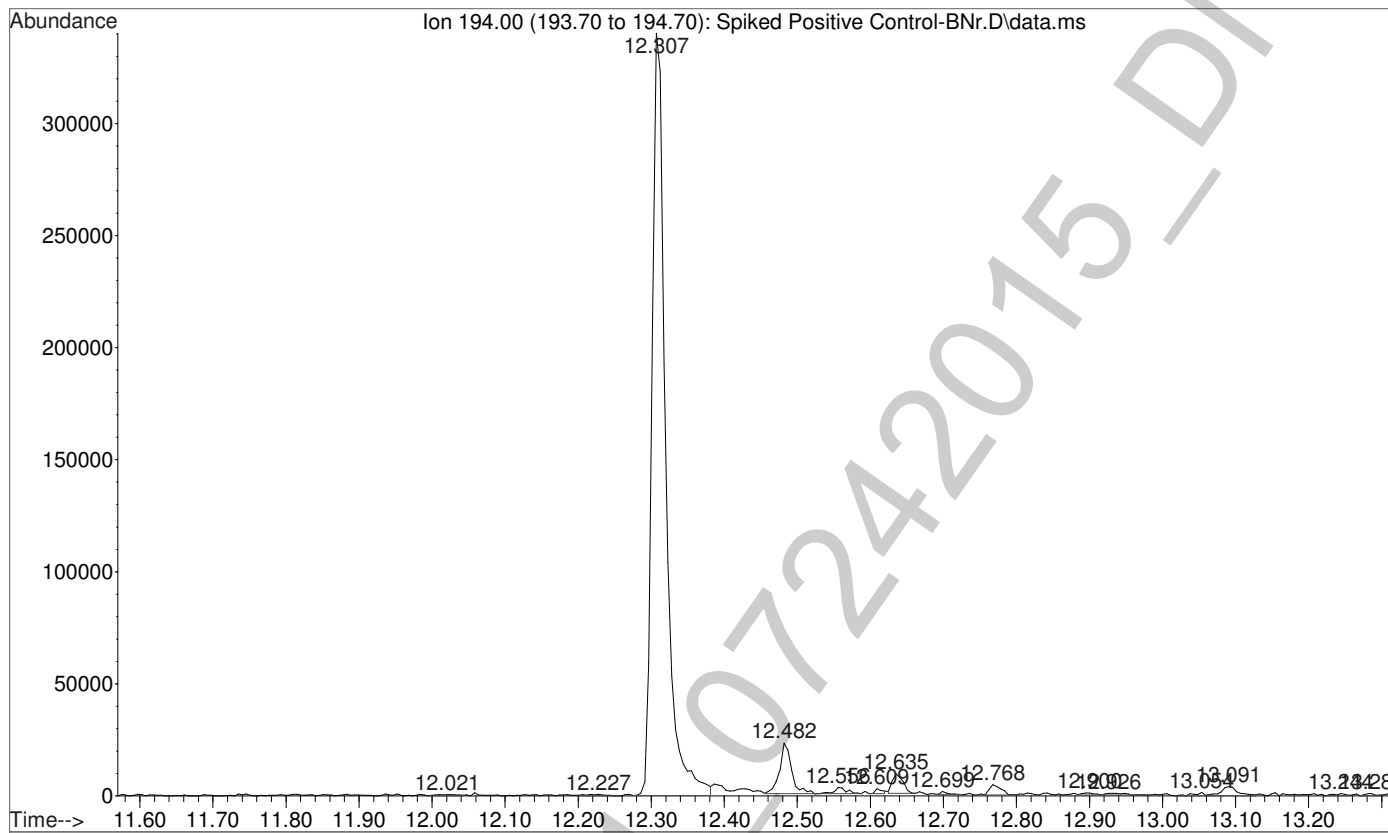



File :C:\gcms\1\data\Blood\072415\Reinjection Longer GC Method\Spi
... ked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 24 Jul 2015 14:21 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

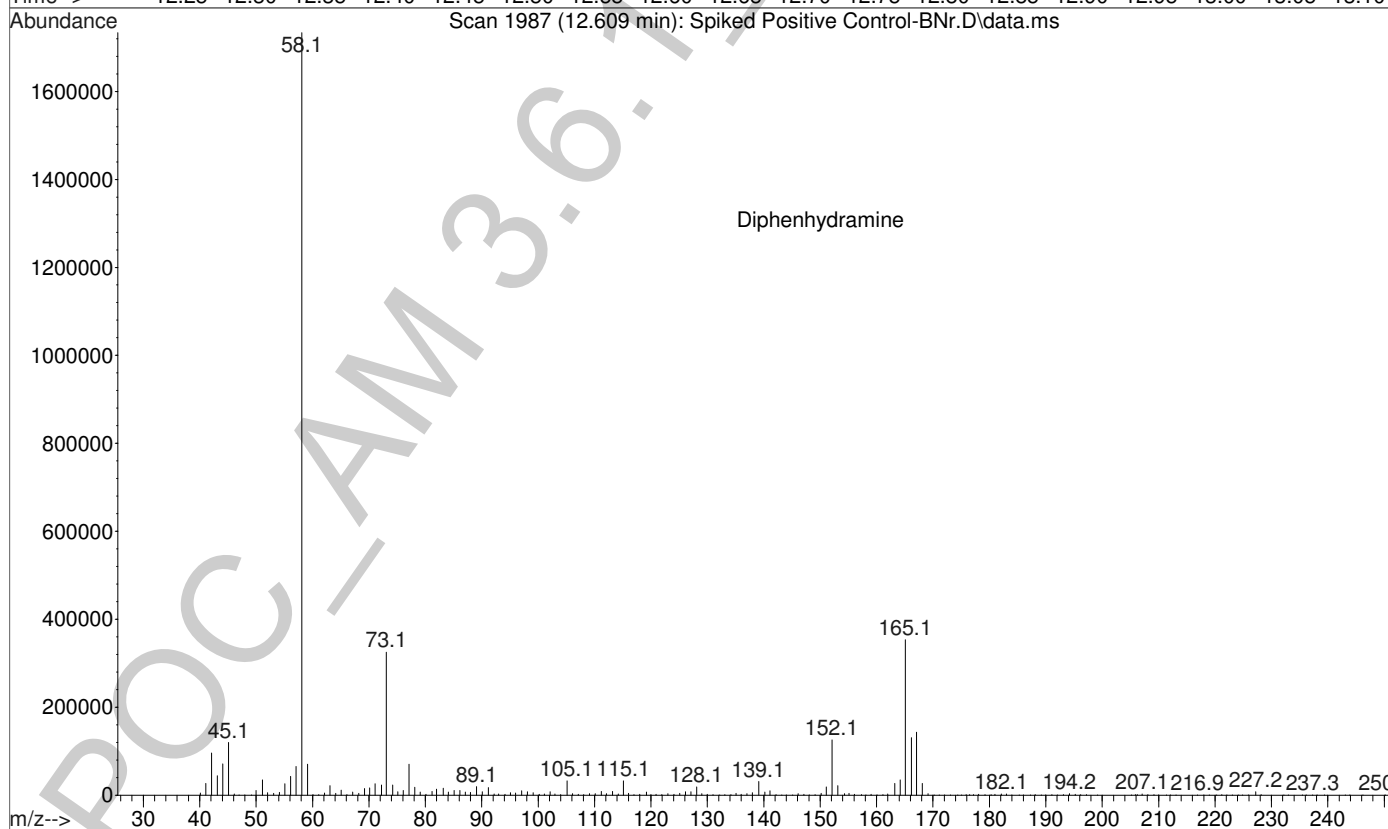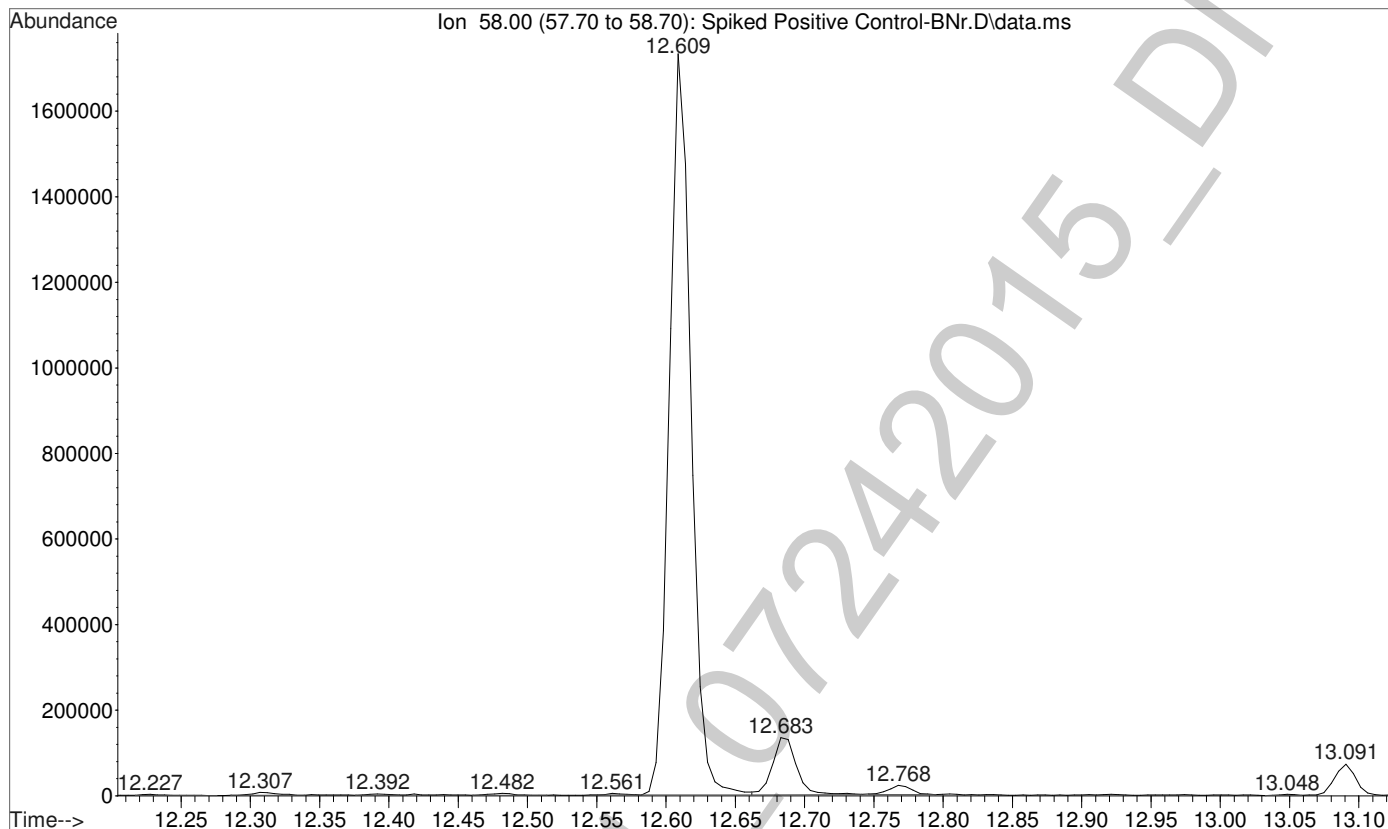



File :C:\gcms\1\data\Blood\072415\Reinjection Longer GC Method\Spiked Positive Control-BNr.D
...
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 24 Jul 2015 14:21 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

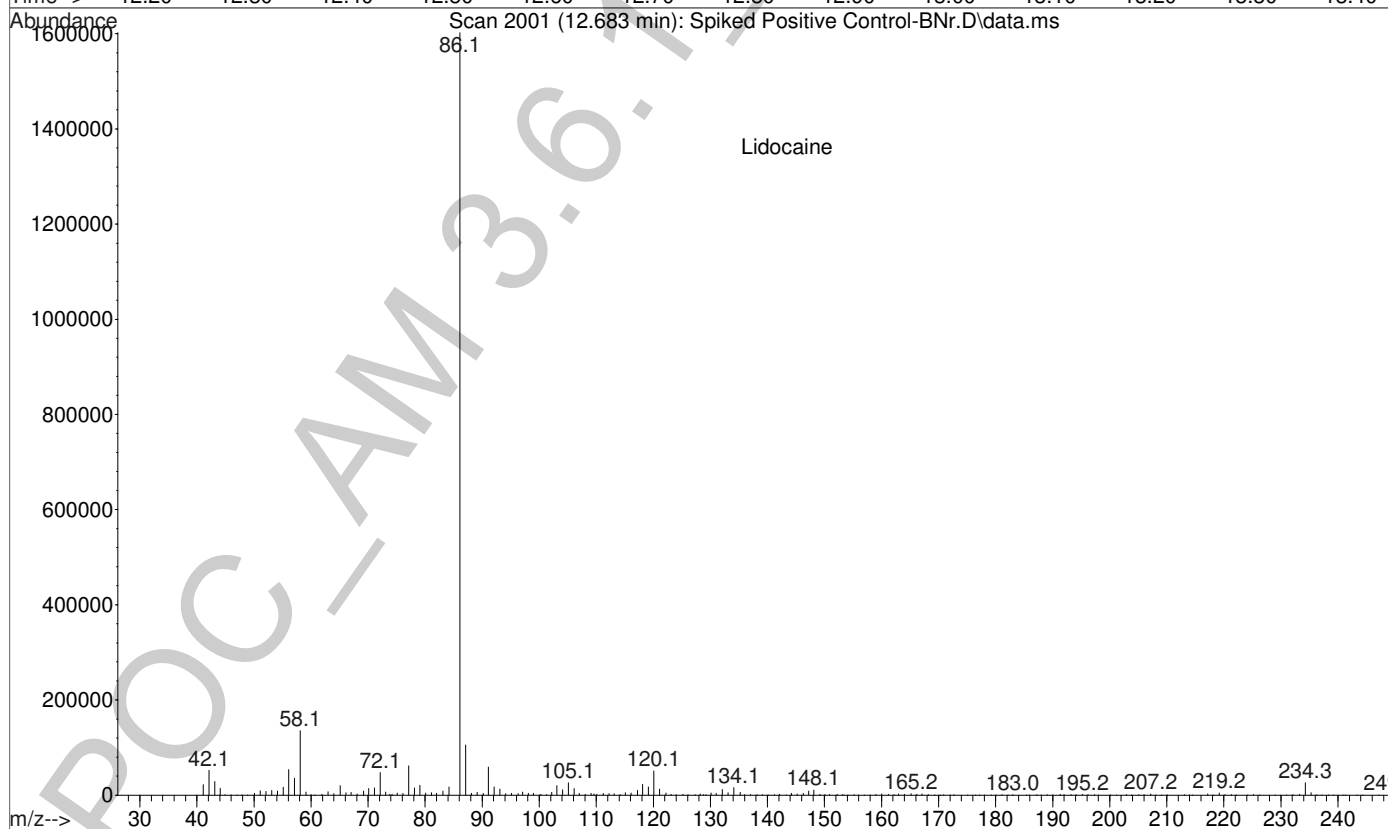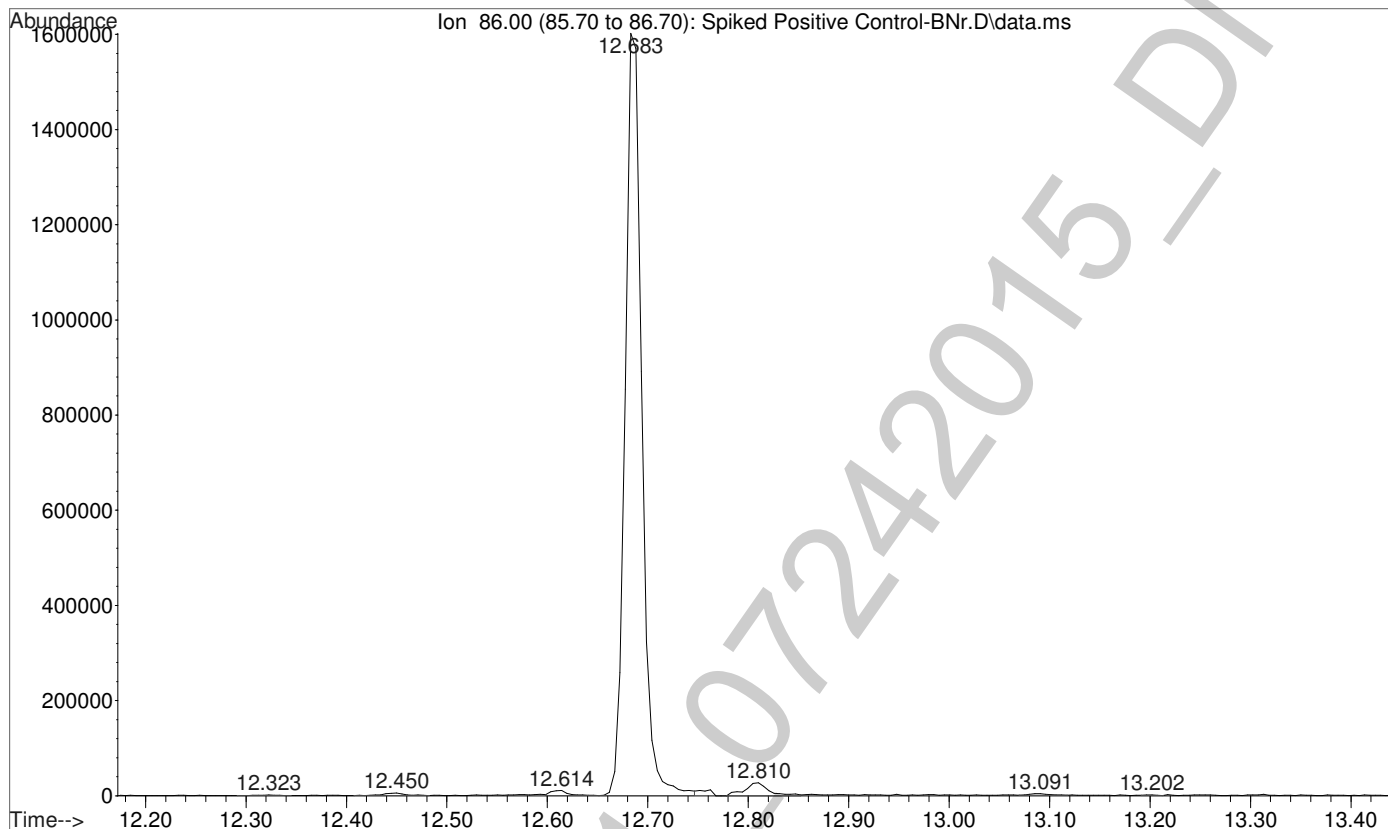



File :C:\gcms\1\data\Blood\072415\Reinjection Longer GC Method\Spiked Positive Control-BNr.D
...
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 24 Jul 2015 14:21 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

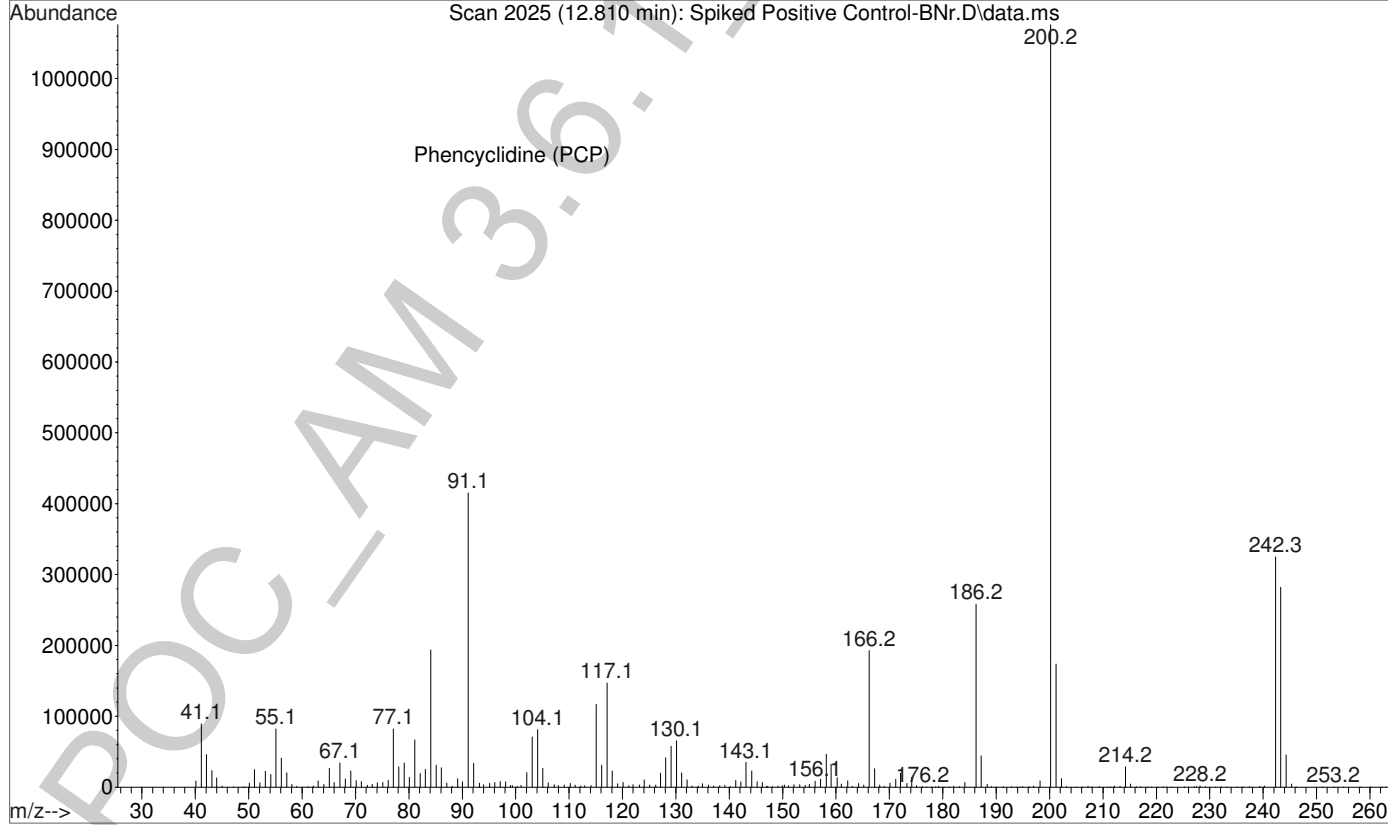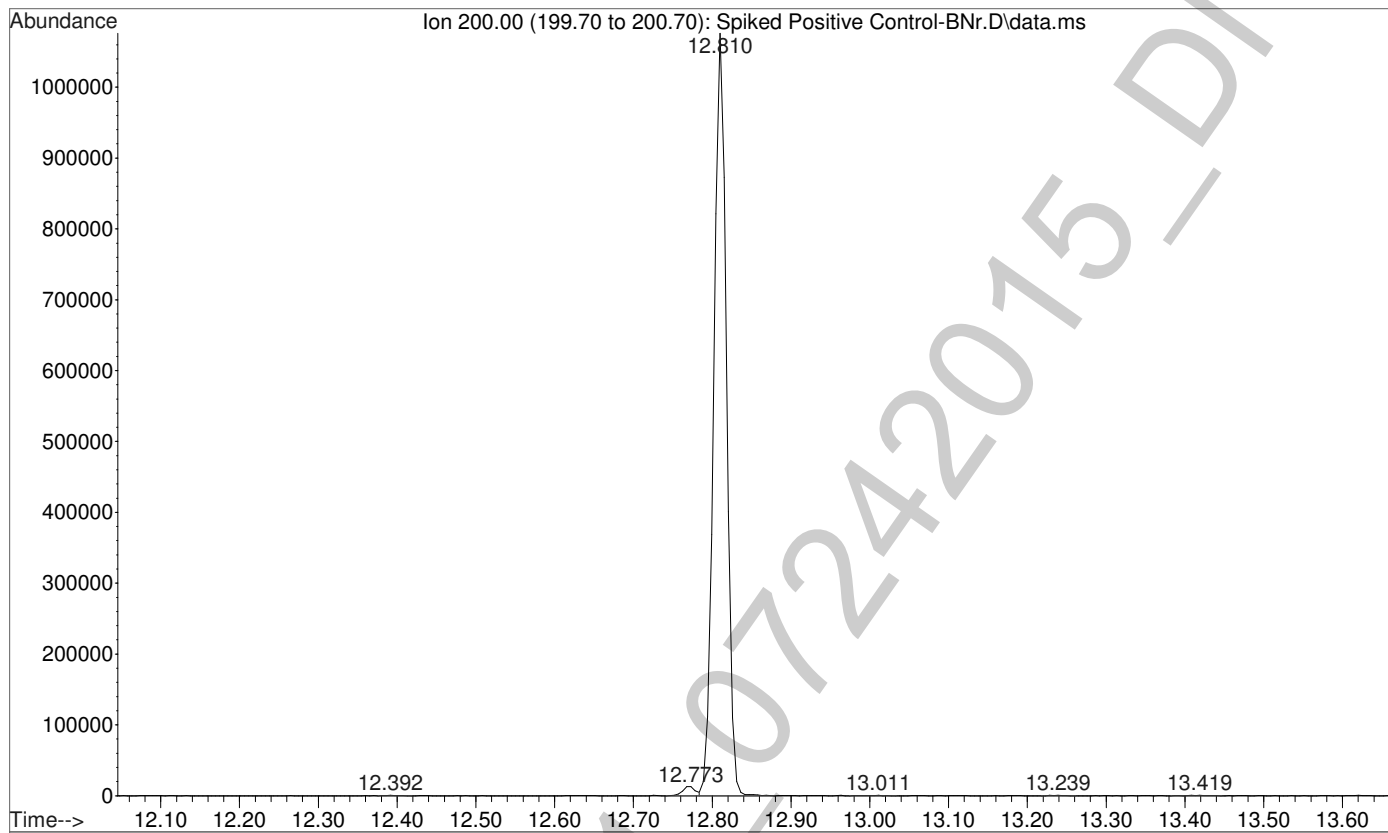



File :C:\gcms\1\data\Blood\072415\Reinjection Longer GC Method\Spi
... ked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 24 Jul 2015 14:21 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

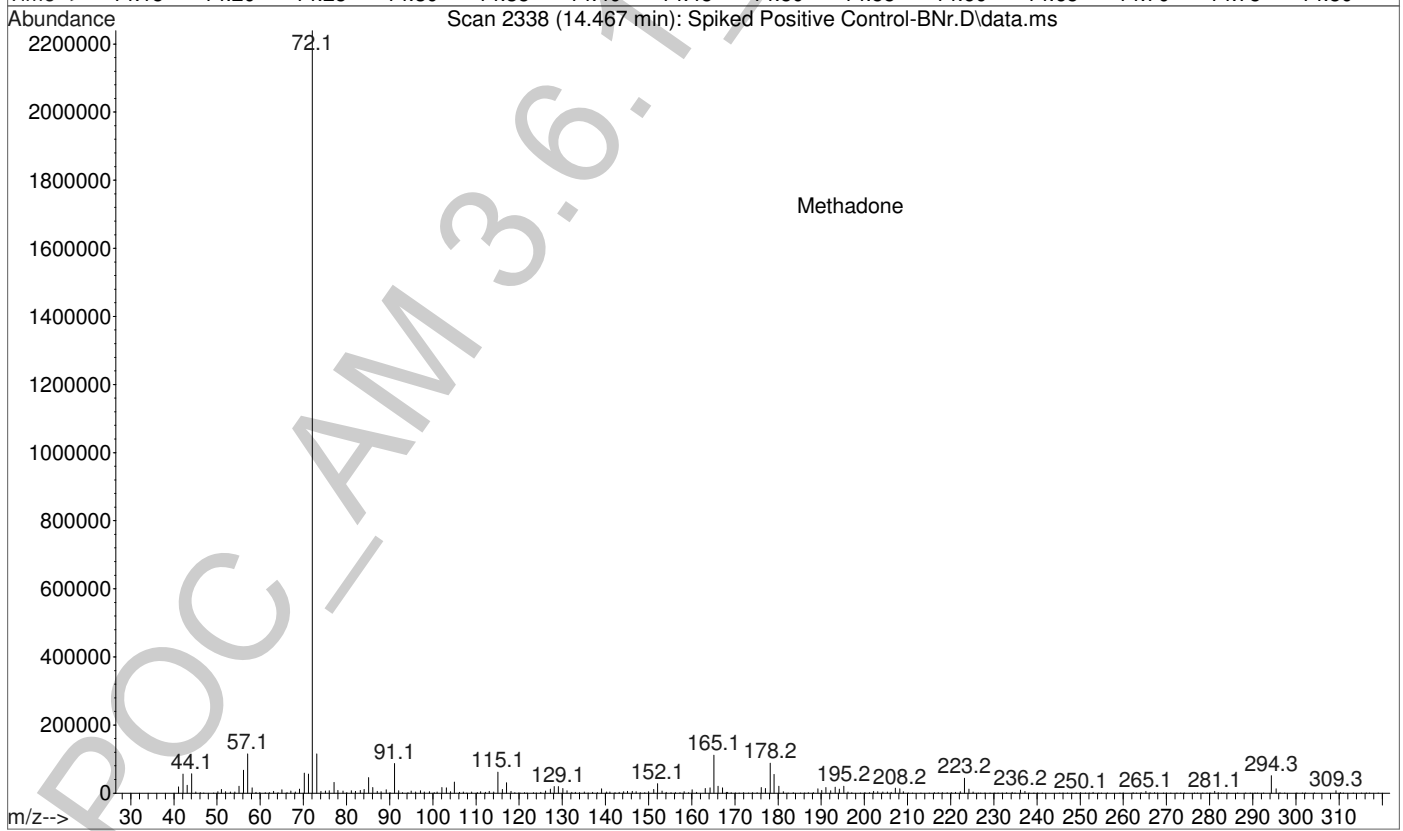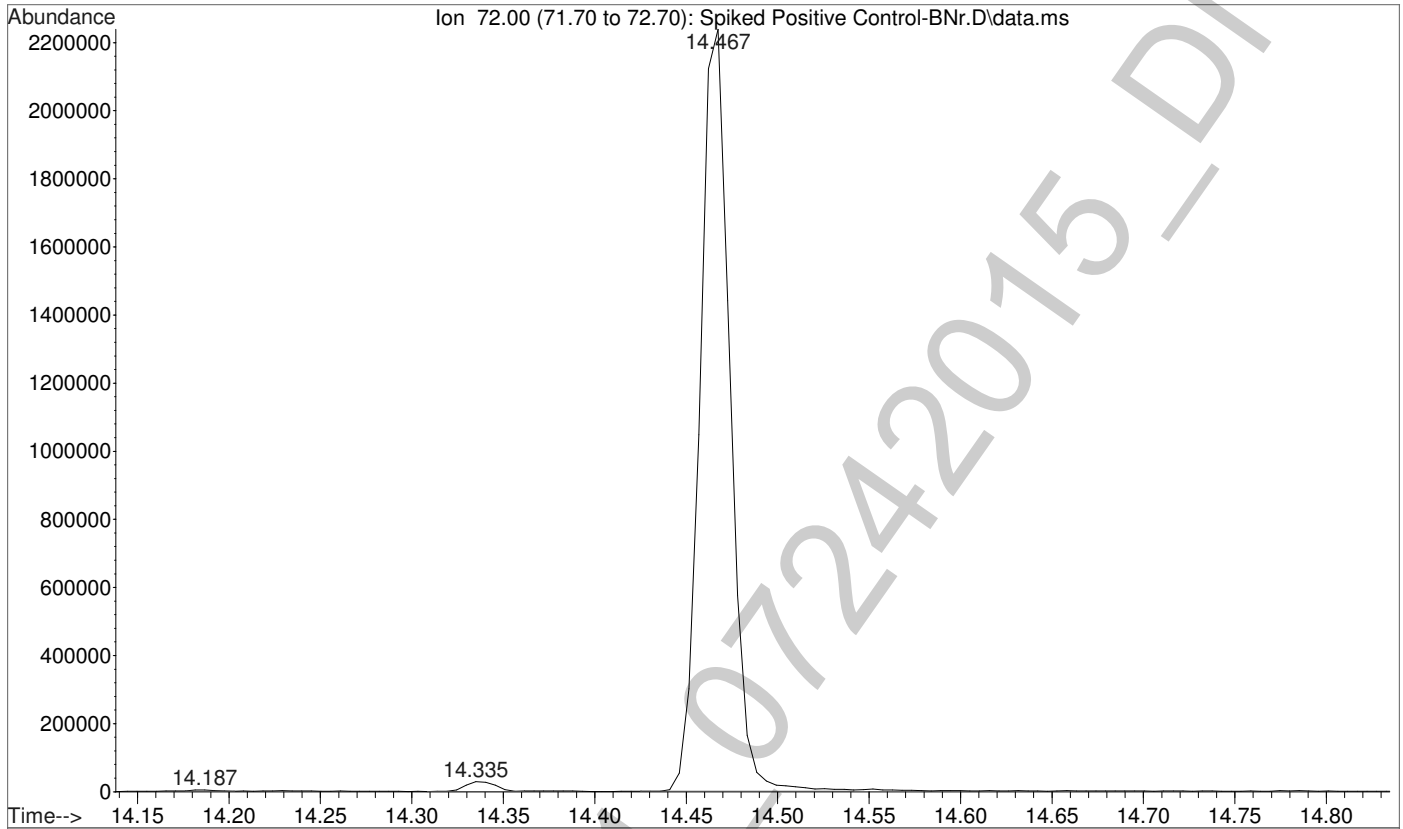



File :C:\gcms\1\data\Blood\072415\Reinjection Longer GC Method\Spi
... ked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 24 Jul 2015 14:21 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

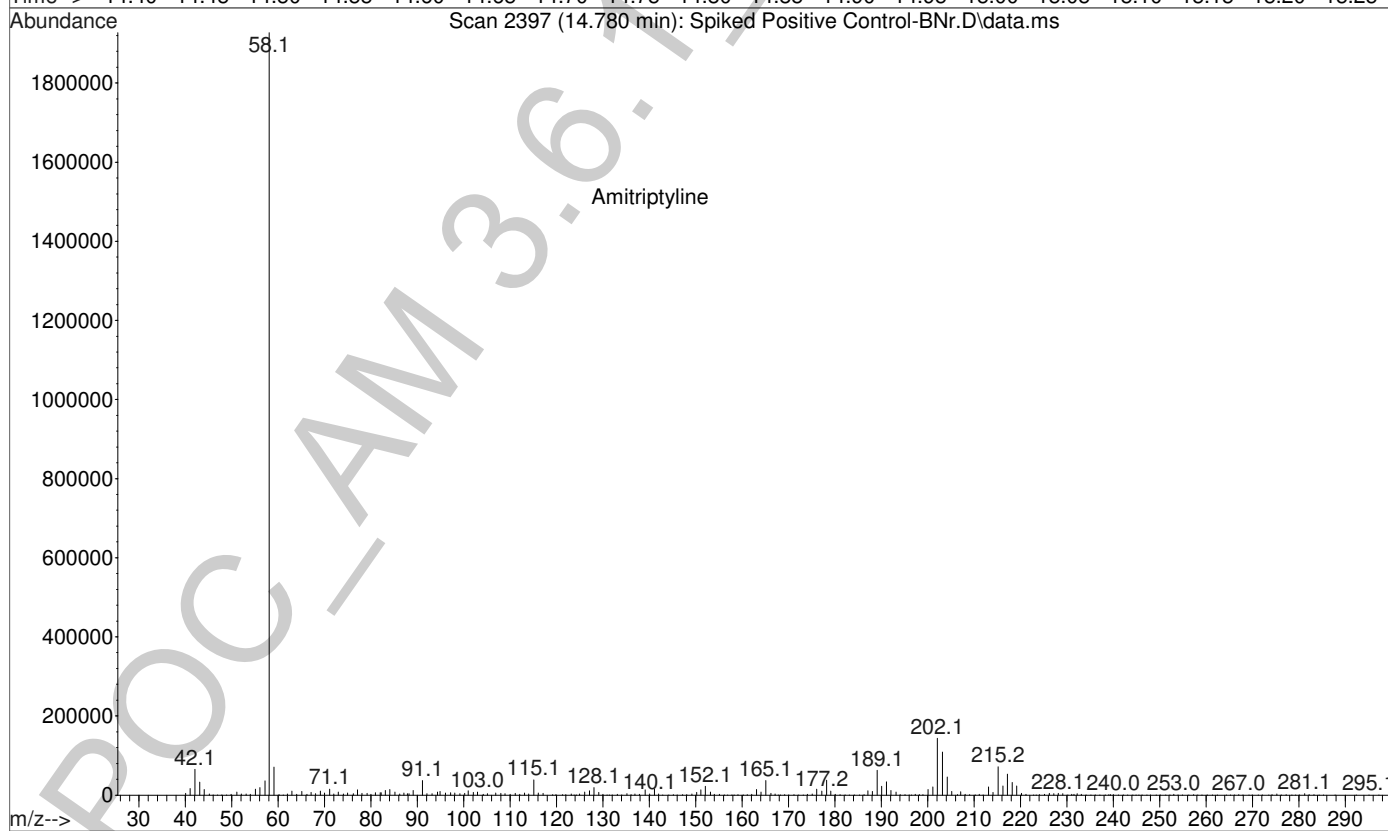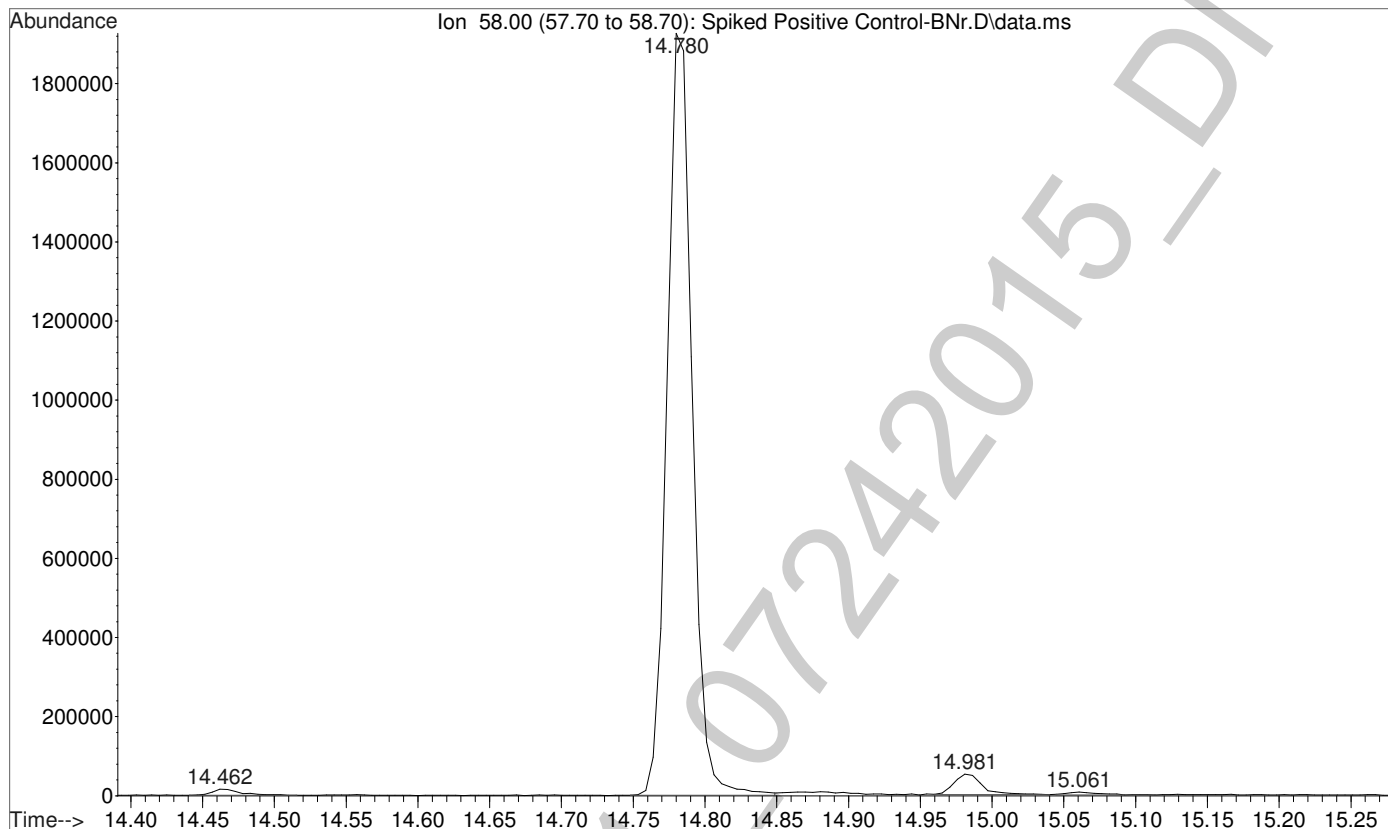



File :C:\gcms\1\data\Blood\072415\Reinjection Longer GC Method\Spi
... ked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 24 Jul 2015 14:21 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

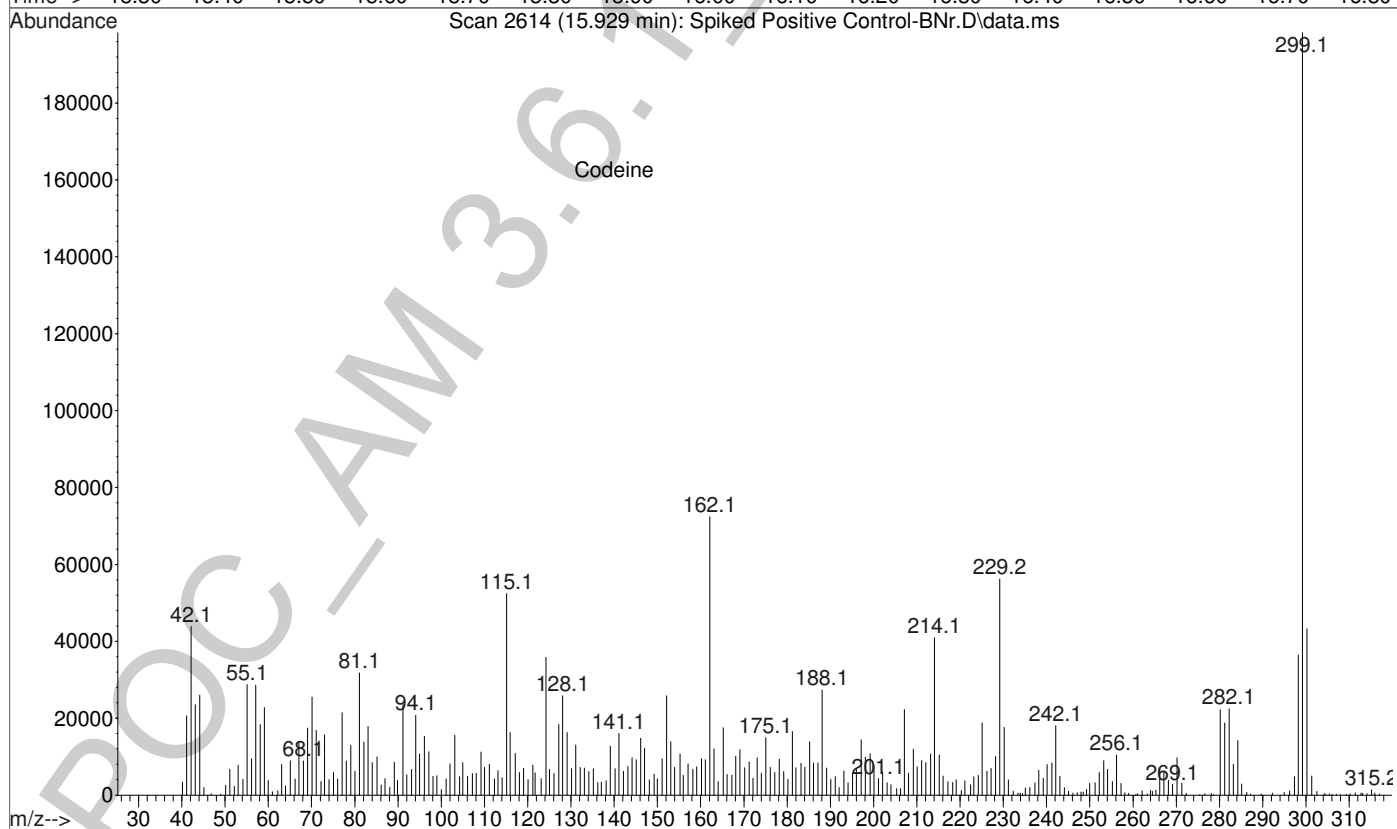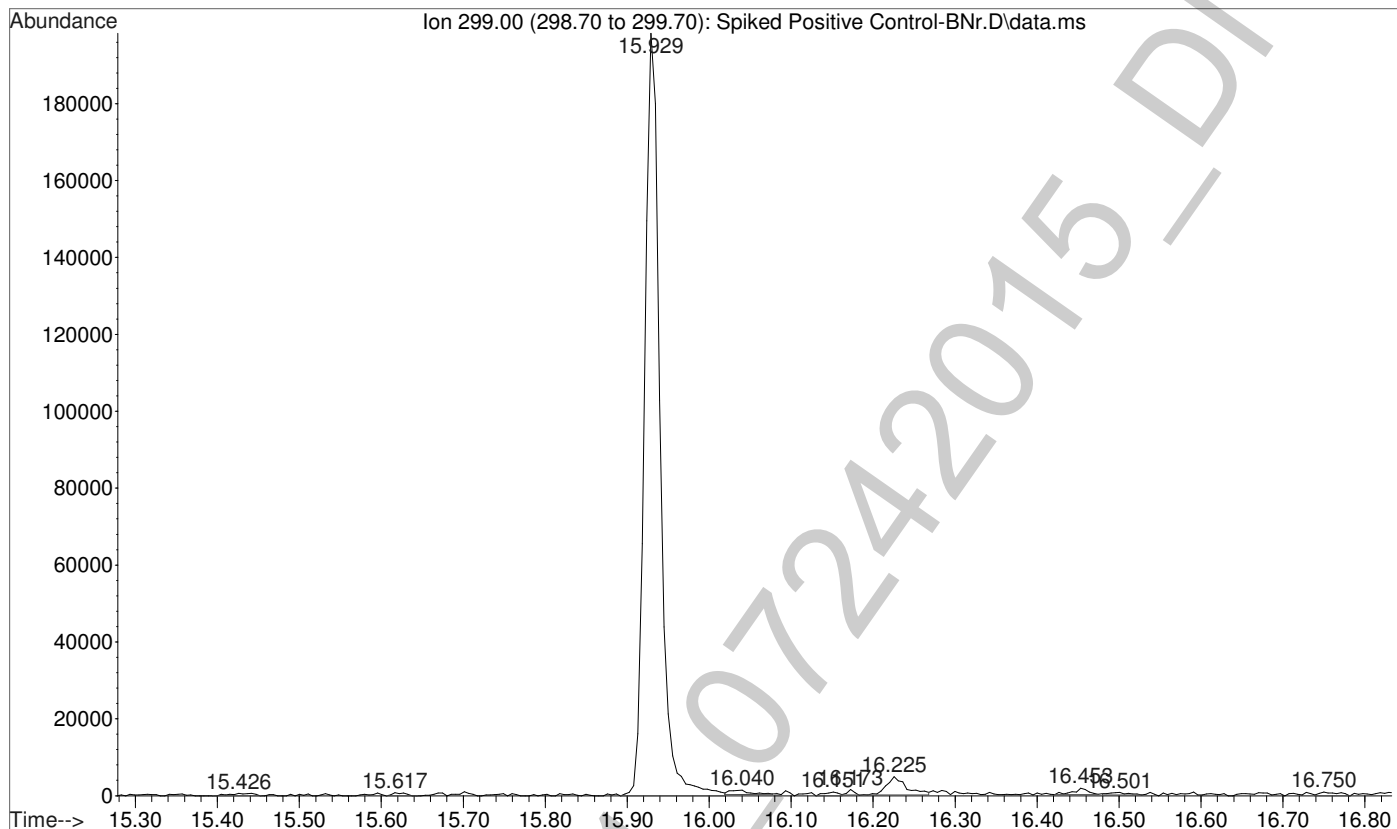



File :C:\gcms\1\data\Blood\072415\Reinjection Longer GC Method\Spi
... ked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 24 Jul 2015 14:21 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

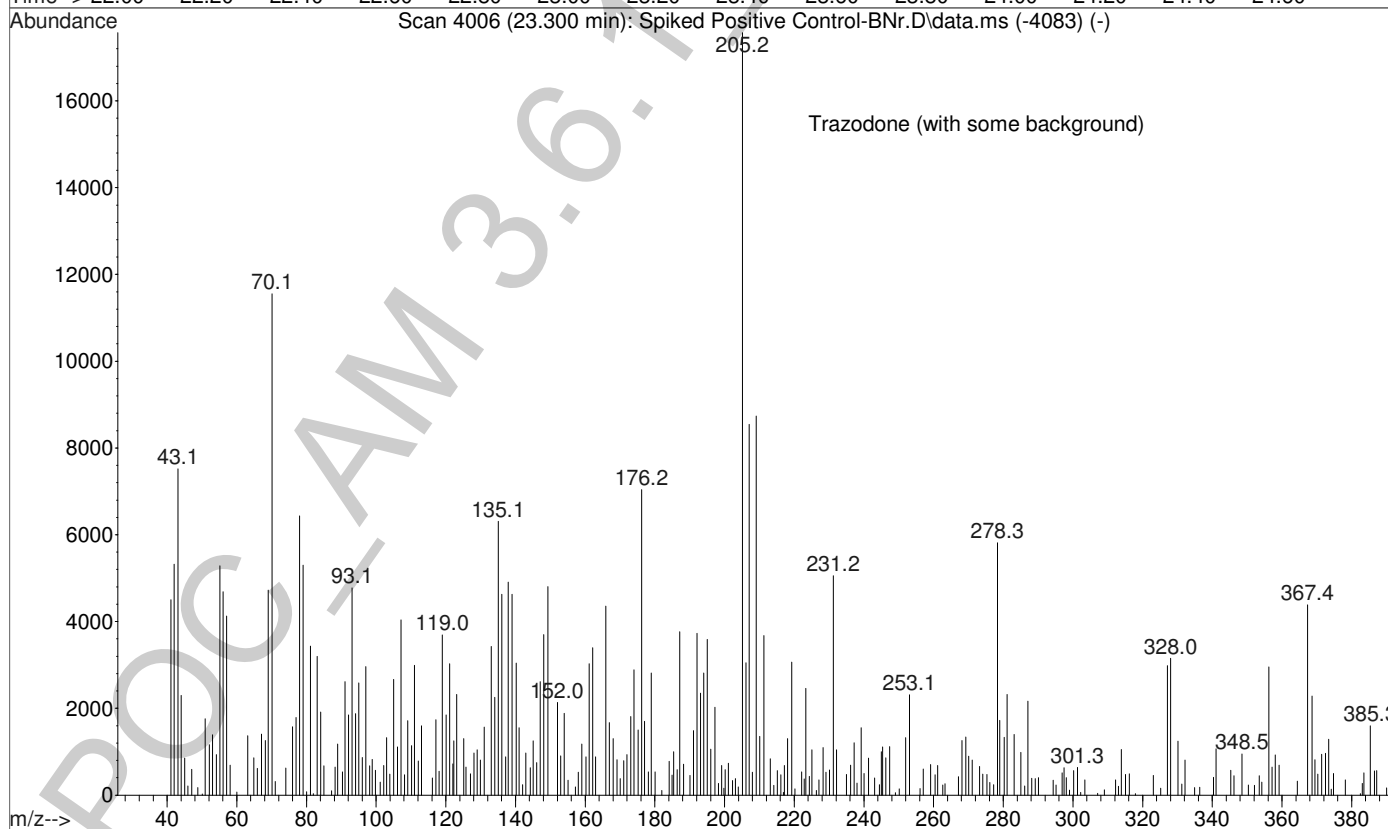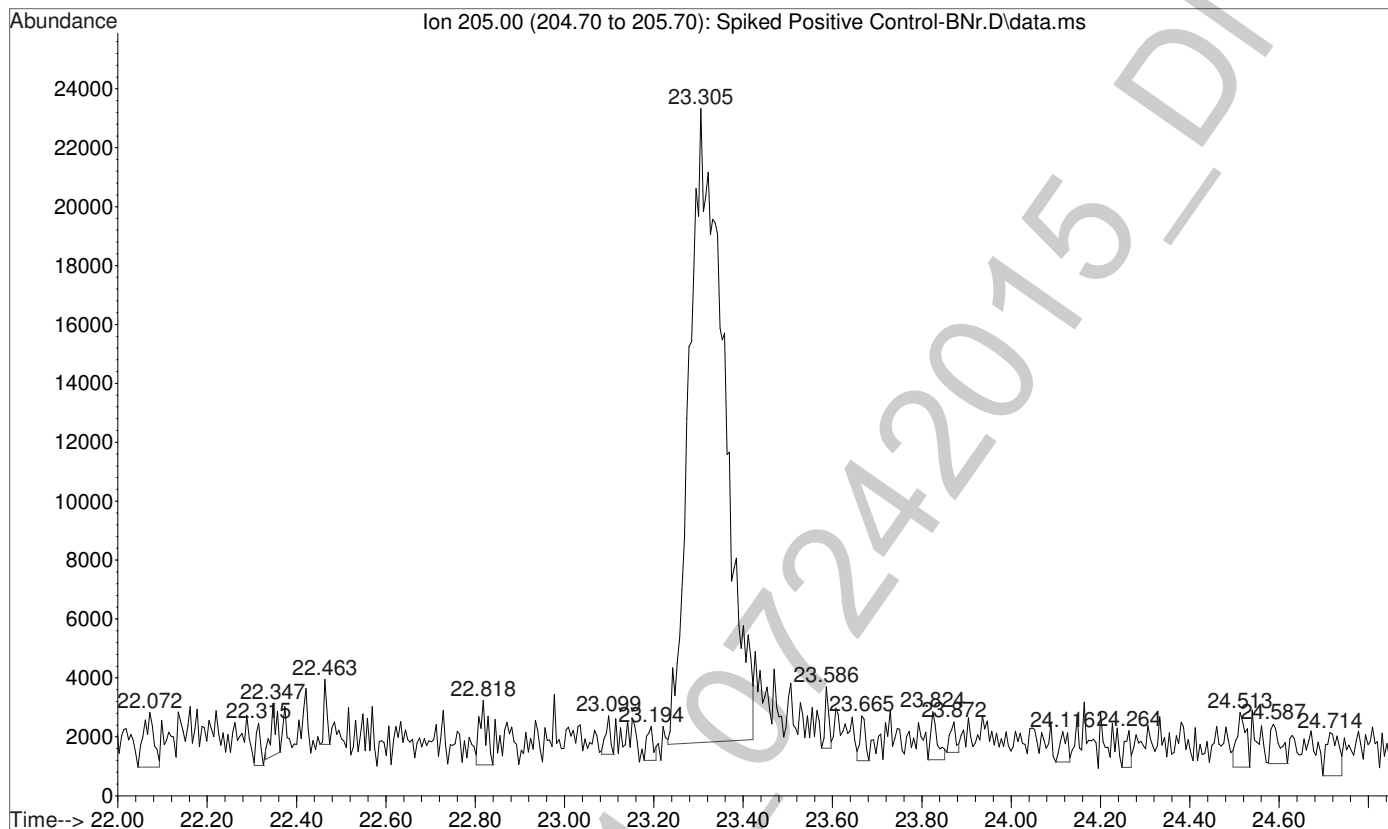

File :C:\gcms\1\data\Blood\072415\Reinjection Longer GC Method\prb
... LK2r.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 24 Jul 2015 14:55 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Solvent Blank
Misc Info : Chloroform

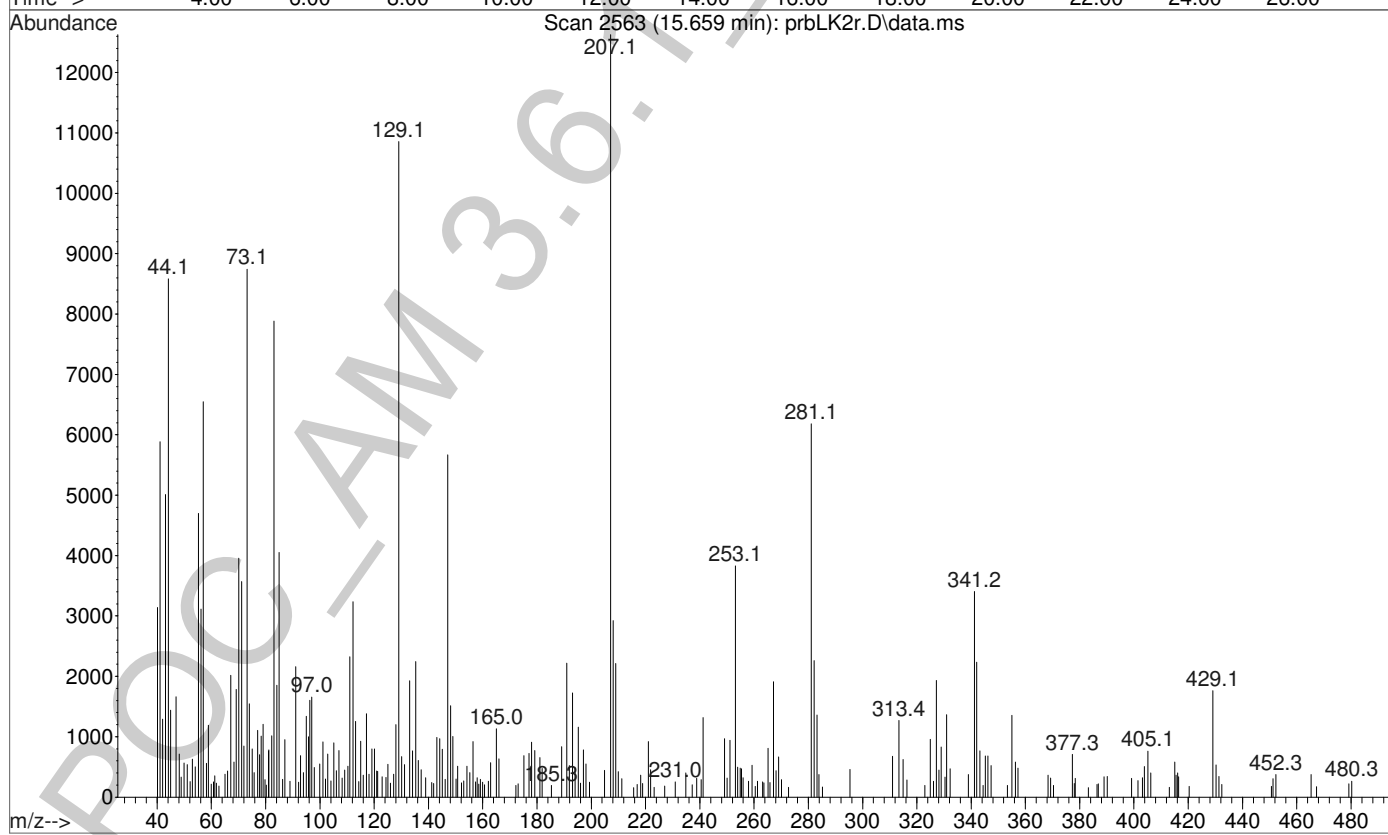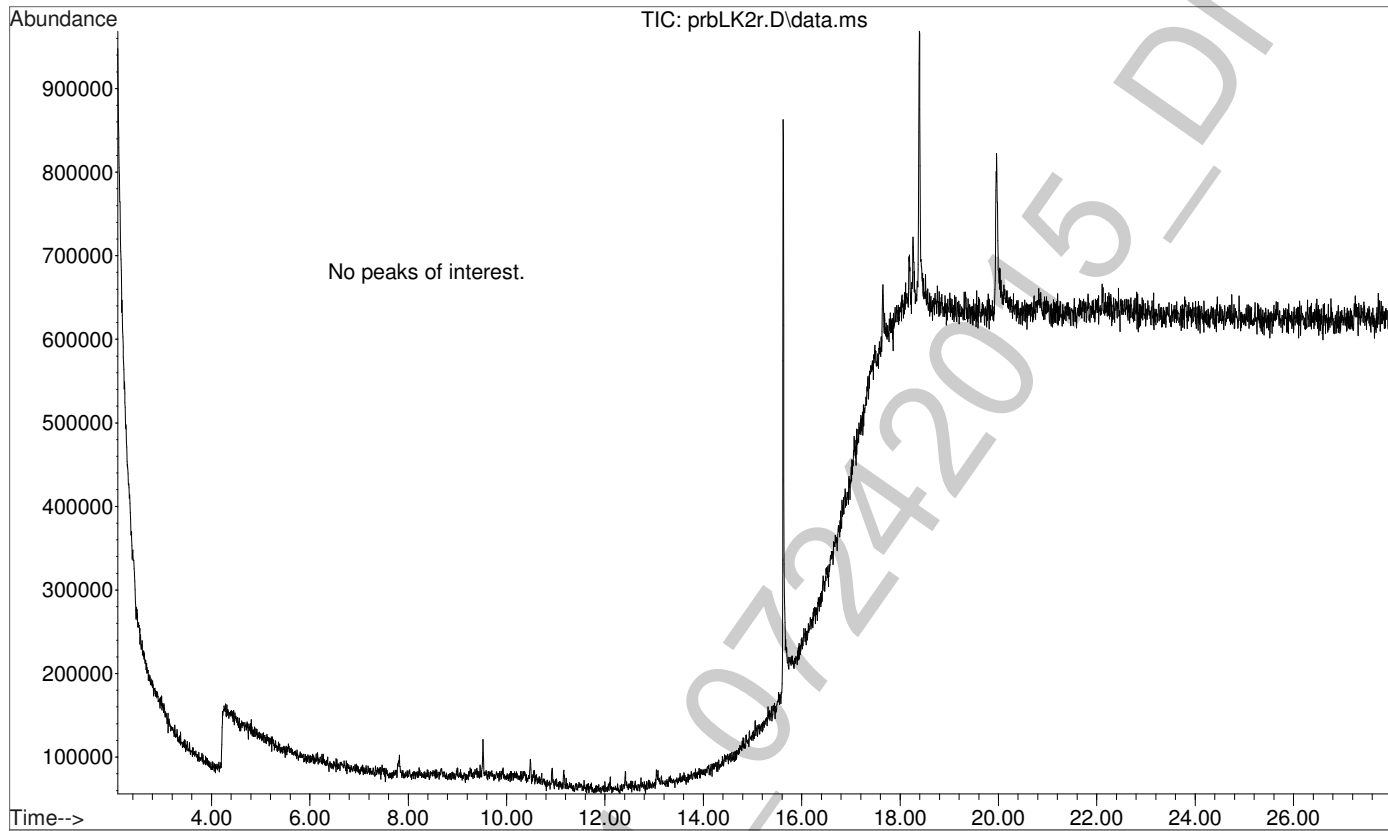

File :C:\gcms\1\data\Blood\072415\Reinjection Longer GC Method\POS
... TBLKr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 26 Jul 2015 22:54 using AcqMethod BNSB120510.M
Sample Name: BLK
Misc Info : Chloroform

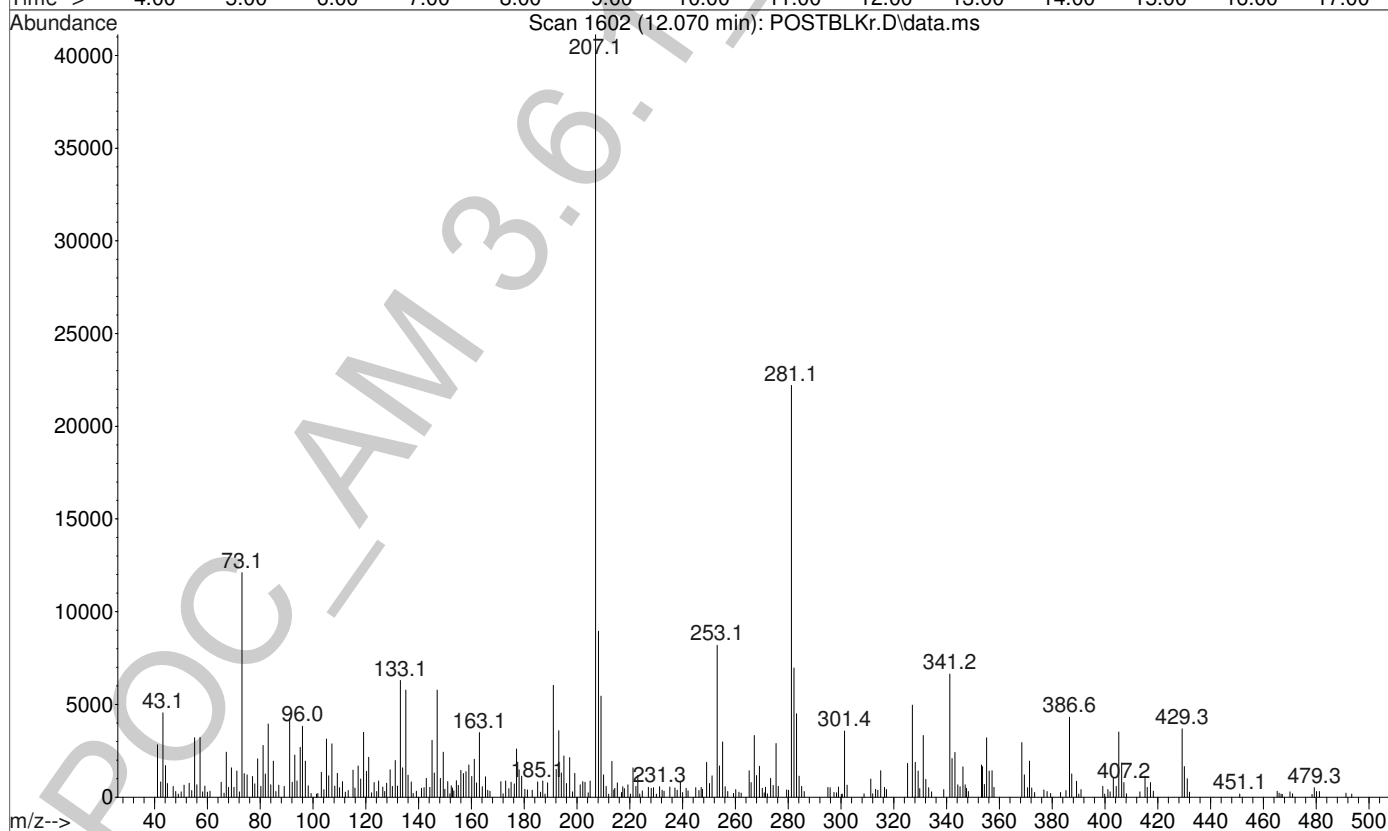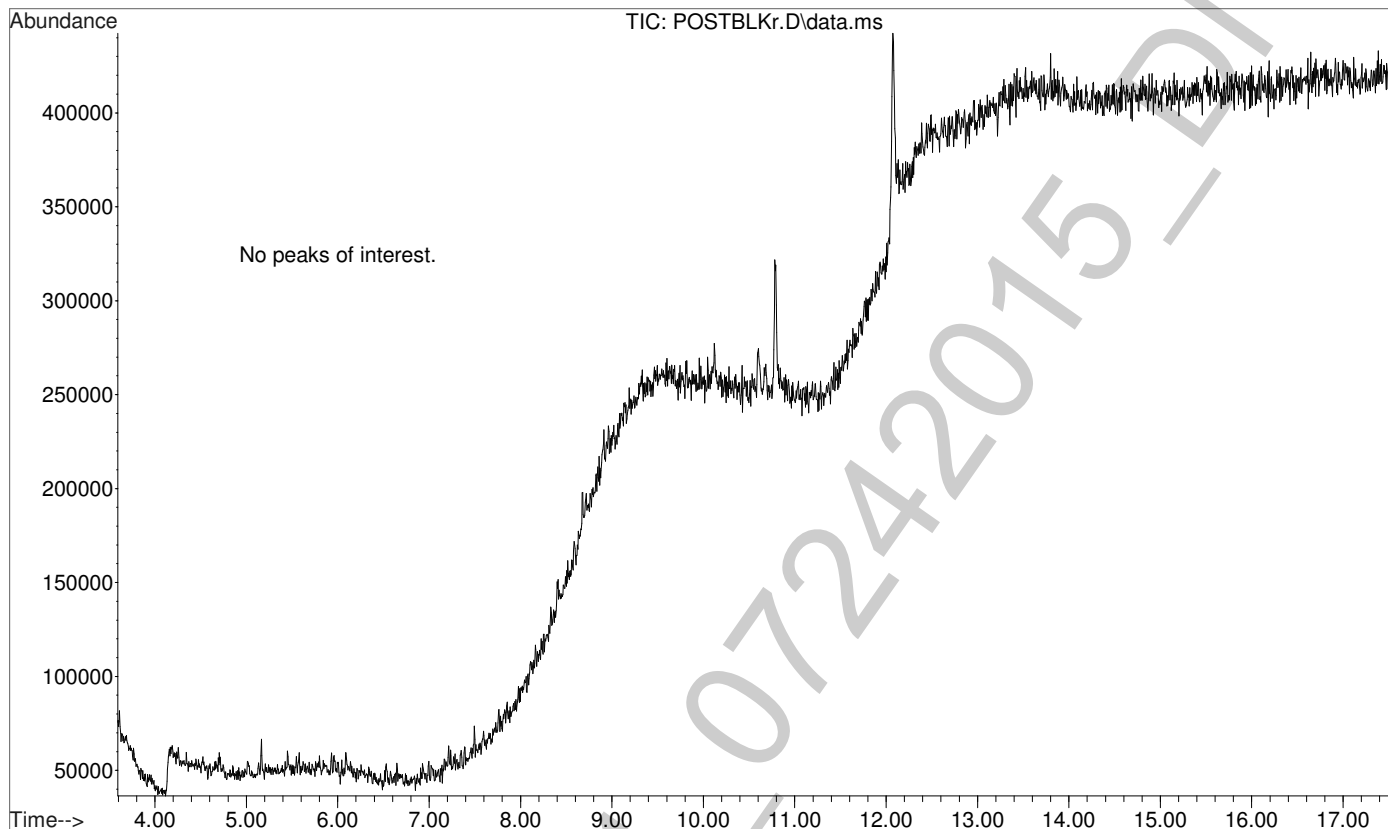

File :C:\gcms\1\data\Blood\072415\AFTER.D
Operator : ISP\datastor
Acquired : 26 Jul 2015 23:16 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: BLK
Misc Info : Chloroform
Vial Number: 68

