
























reviewed 11-5-15 by BAW

Bylee

10/27/2015


Worklist: 880

<u>LAB CASE</u>	<u>ITEM</u>	<u>TASK ID</u>	<u>DESCRIPTION</u>	
C2015-1664	1	41437	3.6.1 Blood base neutral confirr	
C2015-1665	1	41441	3.6.1 Blood base neutral confirr	
C2015-1665	2	41897	3.6.1 Blood base neutral confirr	
M2015-2734	3	40179	3.6.1 Blood base neutral confirr	
M2015-2859	1	39376	3.6.1 Blood base neutral confirr	
M2015-2903	2	41722	3.6.1 Blood base neutral confirr	
M2015-3126	1	40496	3.6.1 Blood base neutral confirr	
M2015-3149	1	40624	3.6.1 Blood base neutral confirr	
M2015-3177	1	40726	3.6.1 Blood base neutral confirr	
M2015-3180	1	40735	3.6.1 Blood base neutral confirr	
M2015-3364	1	43391	3.6.1 Blood base neutral confirr	
M2015-3364	2	41623	3.6.1 Blood base neutral confirr	
M2015-3430	1	41959	3.6.1 Blood base neutral confirr	
P2015-1998	2	41250	3.6.1 Blood base neutral confirr	
P2015-2006	1	40984	3.6.1 Blood base neutral confirr	
P2015-2035	1	41376	3.6.1 Blood base neutral confirr	
P2015-2088	1	43426	3.6.1 Blood base neutral confirr	
P2015-2088	2	43429	3.6.1 Blood base neutral confirr	
P2015-2088	3	43428	3.6.1 Blood base neutral confirr	
P2015-2128	1	42161	3.6.1 Blood base neutral confirr	
P2015-2189	1	42612	3.6.1 Blood base neutral confirr	
P2015-2190	1	42615	3.6.1 Blood base neutral confirr	
P2015-2191	1	42679	3.6.1 Blood base neutral confirr	

Reviewed by DND on 11/06/2015. *DE*

Worklist: 880

<u>LAB_CASE</u>	<u>ITEM</u>	<u>TASK_ID</u>	<u>DESCRIPTION</u>
P2015-2192	1	42682	3.6.1 Blood base neutral confirr
P2015-2208	1	42801	3.6.1 Blood base neutral confirr

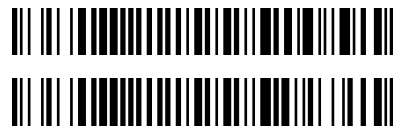

simulate_sequence.log
Simulate Run Sequence Thu Oct 15 12:29:40 2015

Instrument Name: Major Mass Spec
Sequence File: C:\Users\ISPuser\Desktop\Sequences\CS-BNSB101515.sequence.xml
Comment: MassHunter sequence
Operator: ISP\datastor
Data Path: D:\DATA\CDS\2015\101515\
Method Path: D:\MassHunter\GCMS\1\methods\

Line	Type	Vials	DataFile	Sample Name
Acquisition Method: BNSB120510.M				
1)	Sample	100	Prerun Solvent Blank	Pre-run Solvent Blank
2)	Sample	1	Negative Control-BN	Negative Control -
...	0689			
3)	Sample	2	Spiked Positive Control-BN	Positive Control
4)	Sample	99	prBLK2	Solvent Blank
Acquisition Method: GBT092509-Delta EMV.M				
5)	Sample	100	Prerun Solvent Blankr	Pre-run Solvent Blank
6)	Sample	1	Negative Control-BNr	Negative Control -
...	0689			
7)	Sample	2	Spiked Positive Control-BNr	Positive Control
8)	Sample	99	prBLK2r	Solvent Blank
Acquisition Method: BNSB120510.M				
9)	Sample	98	C2015-1664-1-BNBLK	Lab No.: C2015-1664-1
10)	Sample	3	C2015-1664-1-BN	Lab No.: C2015-1664-1
11)	Sample	97	C2015-1665-1-BNBLK	Lab No.: C2015-1665-1
12)	Sample	4	C2015-1665-1-BN	Lab No.: C2015-1665-1
13)	Sample	96	C2015-1665-2-BNBLK	Lab No.: C2015-1665-2
14)	Sample	5	C2015-1665-2-BN	Lab No.: C2015-1665-2
15)	Sample	95	M2015-2734-3-BNBLK	Lab No.: M2015-2734-3
16)	Sample	6	M2015-2734-3-BN	Lab No.: M2015-2734-3
17)	Sample	94	M2015-2859-1-BNBLK	Lab No.: M2015-2859-1
18)	Sample	7	M2015-2859-1-BN	Lab No.: M2015-2859-1
19)	Sample	93	M2015-2903-2-BNBLK	Lab No.: M2015-2903-2
20)	Sample	8	M2015-2903-2-BN	Lab No.: M2015-2903-2
21)	Sample	92	M2015-3126-1-BNBLK	Lab No.: M2015-3126-1
22)	Sample	9	M2015-3126-1-BN	Lab No.: M2015-3126-1
23)	Sample	91	M2015-3149-1-BNBLK	Lab No.: M2015-3149-1
24)	Sample	10	M2015-3149-1-BN	Lab No.: M2015-3149-1
Acquisition Method: GBT092509-Delta EMV.M				
25)	Sample	98	C2015-1664-1-BNBLKr	Lab No.: C2015-1664-1
26)	Sample	3	C2015-1664-1-BNr	Lab No.: C2015-1664-1
27)	Sample	97	C2015-1665-1-BNBLKr	Lab No.: C2015-1665-1
28)	Sample	4	C2015-1665-1-BNr	Lab No.: C2015-1665-1
29)	Sample	96	C2015-1665-2-BNBLKr	Lab No.: C2015-1665-2
30)	Sample	5	C2015-1665-2-BNr	Lab No.: C2015-1665-2
31)	Sample	95	M2015-2734-3-BNBLKr	Lab No.: M2015-2734-3
32)	Sample	6	M2015-2734-3-BNr	Lab No.: M2015-2734-3
33)	Sample	94	M2015-2859-1-BNBLKr	Lab No.: M2015-2859-1
34)	Sample	7	M2015-2859-1-BNr	Lab No.: M2015-2859-1
35)	Sample	93	M2015-2903-2-BNBLKr	Lab No.: M2015-2903-2
36)	Sample	8	M2015-2903-2-BNr	Lab No.: M2015-2903-2
37)	Sample	92	M2015-3126-1-BNBLKr	Lab No.: M2015-3126-1
38)	Sample	9	M2015-3126-1-BNr	Lab No.: M2015-3126-1
39)	Sample	91	M2015-3149-1-BNBLKr	Lab No.: M2015-3149-1
40)	Sample	10	M2015-3149-1-BNr	Lab No.: M2015-3149-1
Acquisition Method: BNSB120510.M				
41)	Sample	90	M2015-3177-1-BNBLK	Lab No.: M2015-3177-1
42)	Sample	11	M2015-3177-1-BN	Lab No.: M2015-3177-1
43)	Sample	89	M2015-3180-1-BNBLK	Lab No.: M2015-3180-1
44)	Sample	12	M2015-3180-1-BN	Lab No.: M2015-3180-1

simulate_sequence.log			
45) Sample	88	M2015-3364-1-BNBLK	Lab No.: M2015-3364-1
46) Sample	13	M2015-3364-1-BN	Lab No.: M2015-3364-1
47) Sample	87	M2015-3364-2-BNBLK	Lab No.: M2015-3364-2
48) Sample	14	M2015-3364-2-BN	Lab No.: M2015-3364-2
49) Sample	86	M2015-3430-1-BNBLK	Lab No.: M2015-3430-1
50) Sample	15	M2015-3430-1-BN	Lab No.: M2015-3430-1

Acquisition Method: GBT092509-Delta EMV.M			
51) Sample	90	M2015-3177-1-BNBLK	Lab No.: M2015-3177-1
52) Sample	11	M2015-3177-1-BNr	Lab No.: M2015-3177-1
53) Sample	89	M2015-3180-1-BNBLK	Lab No.: M2015-3180-1
54) Sample	12	M2015-3180-1-BNr	Lab No.: M2015-3180-1
55) Sample	88	M2015-3364-1-BNBLK	Lab No.: M2015-3364-1
56) Sample	13	M2015-3364-1-BNr	Lab No.: M2015-3364-1
57) Sample	87	M2015-3364-2-BNBLK	Lab No.: M2015-3364-2
58) Sample	14	M2015-3364-2-BNr	Lab No.: M2015-3364-2
59) Sample	86	M2015-3430-1-BNBLK	Lab No.: M2015-3430-1
60) Sample	15	M2015-3430-1-BNr	Lab No.: M2015-3430-1

Acquisition Method: BNSB120510.M			
61) Sample	85	P2015-1998-2-BNBLK	Lab No.: P2015-1998-2
62) Sample	16	P2015-1998-2-BN	Lab No.: P2015-1998-2
63) Sample	84	P2015-2006-1-BNBLK	Lab No.: P2015-2006-1
64) Sample	17	P2015-2006-1-BN	Lab No.: P2015-2006-1
65) Sample	83	P2015-2035-1-BNBLK	Lab No.: P2015-2035-1
66) Sample	18	P2015-2035-1-BN	Lab No.: P2015-2035-1
67) Sample	82	P2015-2088-1-BNBLK	Lab No.: P2015-2088-1
68) Sample	19	P2015-2088-1-BN	Lab No.: P2015-2088-1
69) Sample	81	P2015-2088-2-BNBLK	Lab No.: P2015-2088-2
70) Sample	20	P2015-2088-2-BN	Lab No.: P2015-2088-2

Acquisition Method: GBT092509-Delta EMV.M			
71) Sample	85	P2015-1998-2-BNBLK	Lab No.: P2015-1998-2
72) Sample	16	P2015-1998-2-BNr	Lab No.: P2015-1998-2
73) Sample	84	P2015-2006-1-BNBLK	Lab No.: P2015-2006-1
74) Sample	17	P2015-2006-1-BNr	Lab No.: P2015-2006-1
75) Sample	83	P2015-2035-1-BNBLK	Lab No.: P2015-2035-1
76) Sample	18	P2015-2035-1-BNr	Lab No.: P2015-2035-1
77) Sample	82	P2015-2088-1-BNBLK	Lab No.: P2015-2088-1
78) Sample	19	P2015-2088-1-BNr	Lab No.: P2015-2088-1
79) Sample	81	P2015-2088-2-BNBLK	Lab No.: P2015-2088-2
80) Sample	20	P2015-2088-2-BNr	Lab No.: P2015-2088-2

Acquisition Method: BNSB120510.M			
81) Sample	80	P2015-2088-3-BNBLK	Lab No.: P2015-2088-3
82) Sample	21	P2015-2088-3-BN	Lab No.: P2015-2088-3
83) Sample	79	P2015-2128-1-BNBLK	Lab No.: P2015-2128-1
84) Sample	22	P2015-2128-1-BN	Lab No.: P2015-2128-1
85) Sample	78	P2015-2189-1-BNBLK	Lab No.: P2015-2189-1
86) Sample	23	P2015-2189-1-BN	Lab No.: P2015-2189-1
87) Sample	77	P2015-2190-1-BNBLK	Lab No.: P2015-2190-1
88) Sample	24	P2015-2190-1-BN	Lab No.: P2015-2190-1
89) Sample	76	P2015-2191-1-BNBLK	Lab No.: P2015-2191-1
90) Sample	25	P2015-2191-1-BN	Lab No.: P2015-2191-1

Acquisition Method: GBT092509-Delta EMV.M			
91) Sample	80	P2015-2088-3-BNBLK	Lab No.: P2015-2088-3
92) Sample	21	P2015-2088-3-BNr	Lab No.: P2015-2088-3
93) Sample	79	P2015-2128-1-BNBLK	Lab No.: P2015-2128-1
94) Sample	22	P2015-2128-1-BNr	Lab No.: P2015-2128-1
95) Sample	78	P2015-2189-1-BNBLK	Lab No.: P2015-2189-1
96) Sample	23	P2015-2189-1-BNr	Lab No.: P2015-2189-1
97) Sample	77	P2015-2190-1-BNBLK	Lab No.: P2015-2190-1
98) Sample	24	P2015-2190-1-BNr	Lab No.: P2015-2190-1
99) Sample	76	P2015-2191-1-BNBLK	Lab No.: P2015-2191-1
100) Sample	25	P2015-2191-1-BNr	Lab No.: P2015-2191-1

Acquisition Method: BNSB120510.M			
----------------------------------	--	--	--

```

simulate_sequence.log
101) Sample      75      P2015-2192-1-BNBLK      Lab No.: P2015-2192-1
102) Sample      26      P2015-2192-1-BN       Lab No.: P2015-2192-1

Acquisition Method: GBT092509-Delta EMV.M
103) Sample      75      P2015-2192-1-BNBLKr   Lab No.: P2015-2192-1
104) Sample      26      P2015-2192-1-BNr     Lab No.: P2015-2192-1

Acquisition Method: BNSB120510.M
105) Sample      74      P2015-2208-1-BNBLK    Lab No.: P2015-2208-1
106) Sample      27      P2015-2208-1-BN      Lab No.: P2015-2208-1

Acquisition Method: GBT092509-Delta EMV.M
107) Sample      74      P2015-2208-1-BNBLKr   Lab No.: P2015-2208-1
108) Sample      27      P2015-2208-1-BNr     Lab No.: P2015-2208-1

Acquisition Method: BNSB120510.M
109) Sample      73      POSTBLK                BLK

Acquisition Method: GBT092509-Delta EMV.M
110) Sample      72      AFTER                  BLK
megabytes Needed: 1515  Space on drive D: 269341
Sequence Verification Done!

```

Analytical Method 3.6.1 & 3.6.7 QA Check List

Run Start Date: 10/15/15

Analyst: CS

(Short GC/MS temperature program)

Positive Control Compound List

- Methamphetamine
- Nicotine
- Meperidine
- Caffeine
- Diphenhydramine
- Lidocaine
- PCP
- Methadone
- Amitriptyline
- Codeine
- Trazodone



Internal Standards

- Benzphetamine
- Papaverine



Optional back extraction **not** performed.
Reconstituted in MeOH.

Phentermine was also added. ٤٣


File :C:\MyFiles\cshrum\Desktop\101515 Data\Prerun Solvent Blank.D
Operator : ISP\datastor
Acquired : 15 Oct 2015 19:32 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Pre-run Solvent Blank
Misc Info : Chloroform
Vial Number: 100

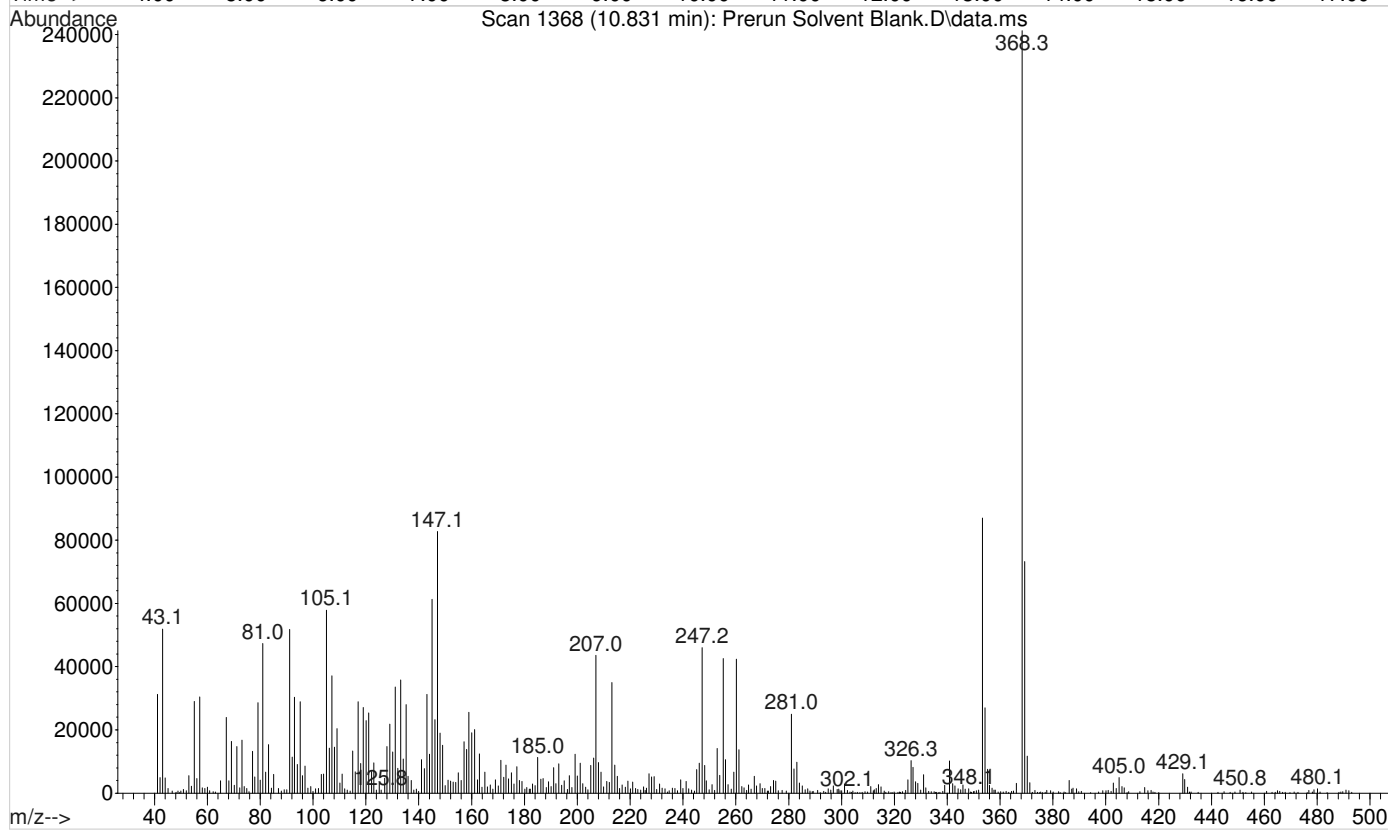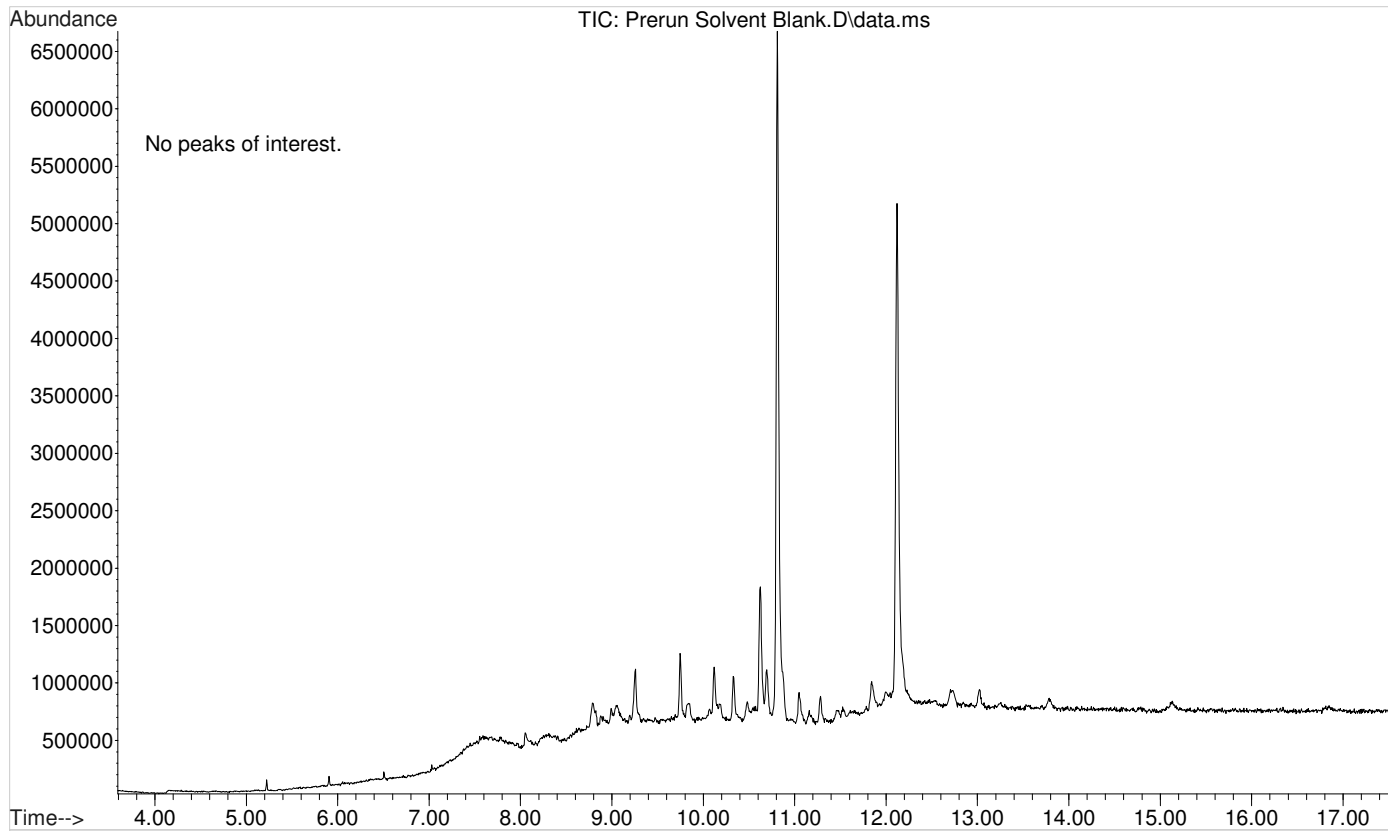



File :C:\MyFiles\cshrum\Desktop\101515 Data\prbLK2.D
Operator : ISP\datastor
Acquired : 15 Oct 2015 20:41 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Solvent Blank
Misc Info : Chloroform
Vial Number: 99

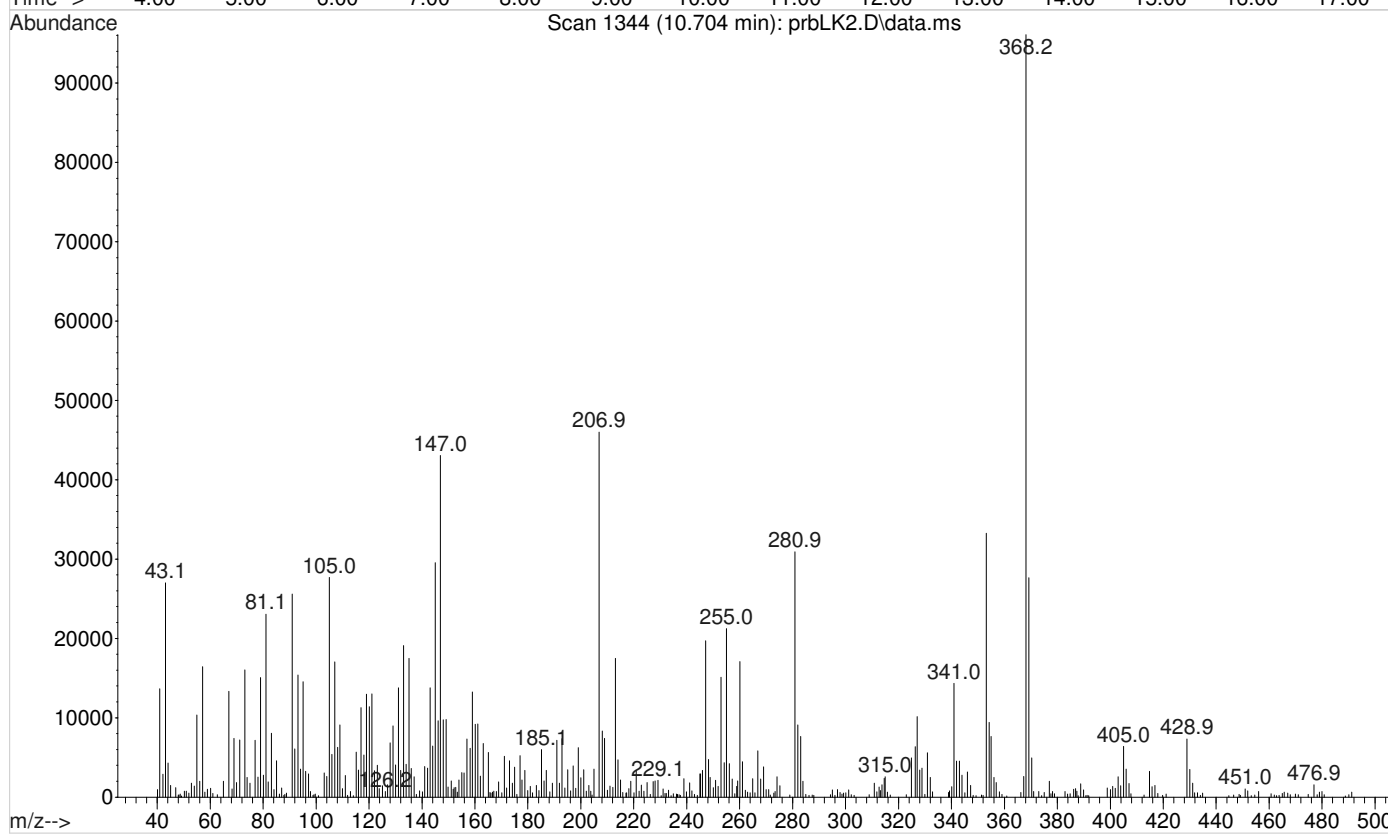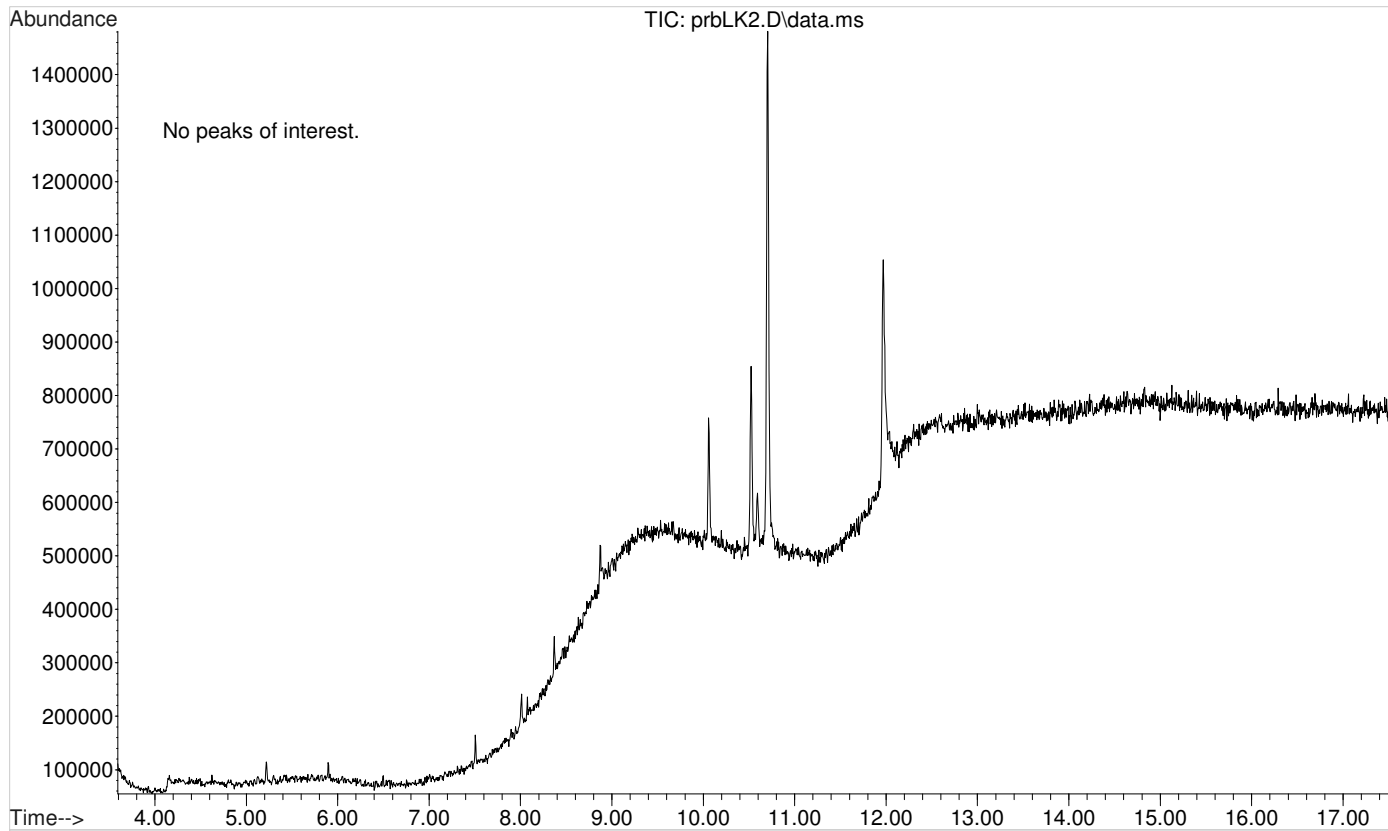



File :C:\MyFiles\cshrum\Desktop\101515 Data\Negative Control-BN.D
Operator : ISP\datastor
Acquired : 15 Oct 2015 19:55 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1
Vial Number: 1

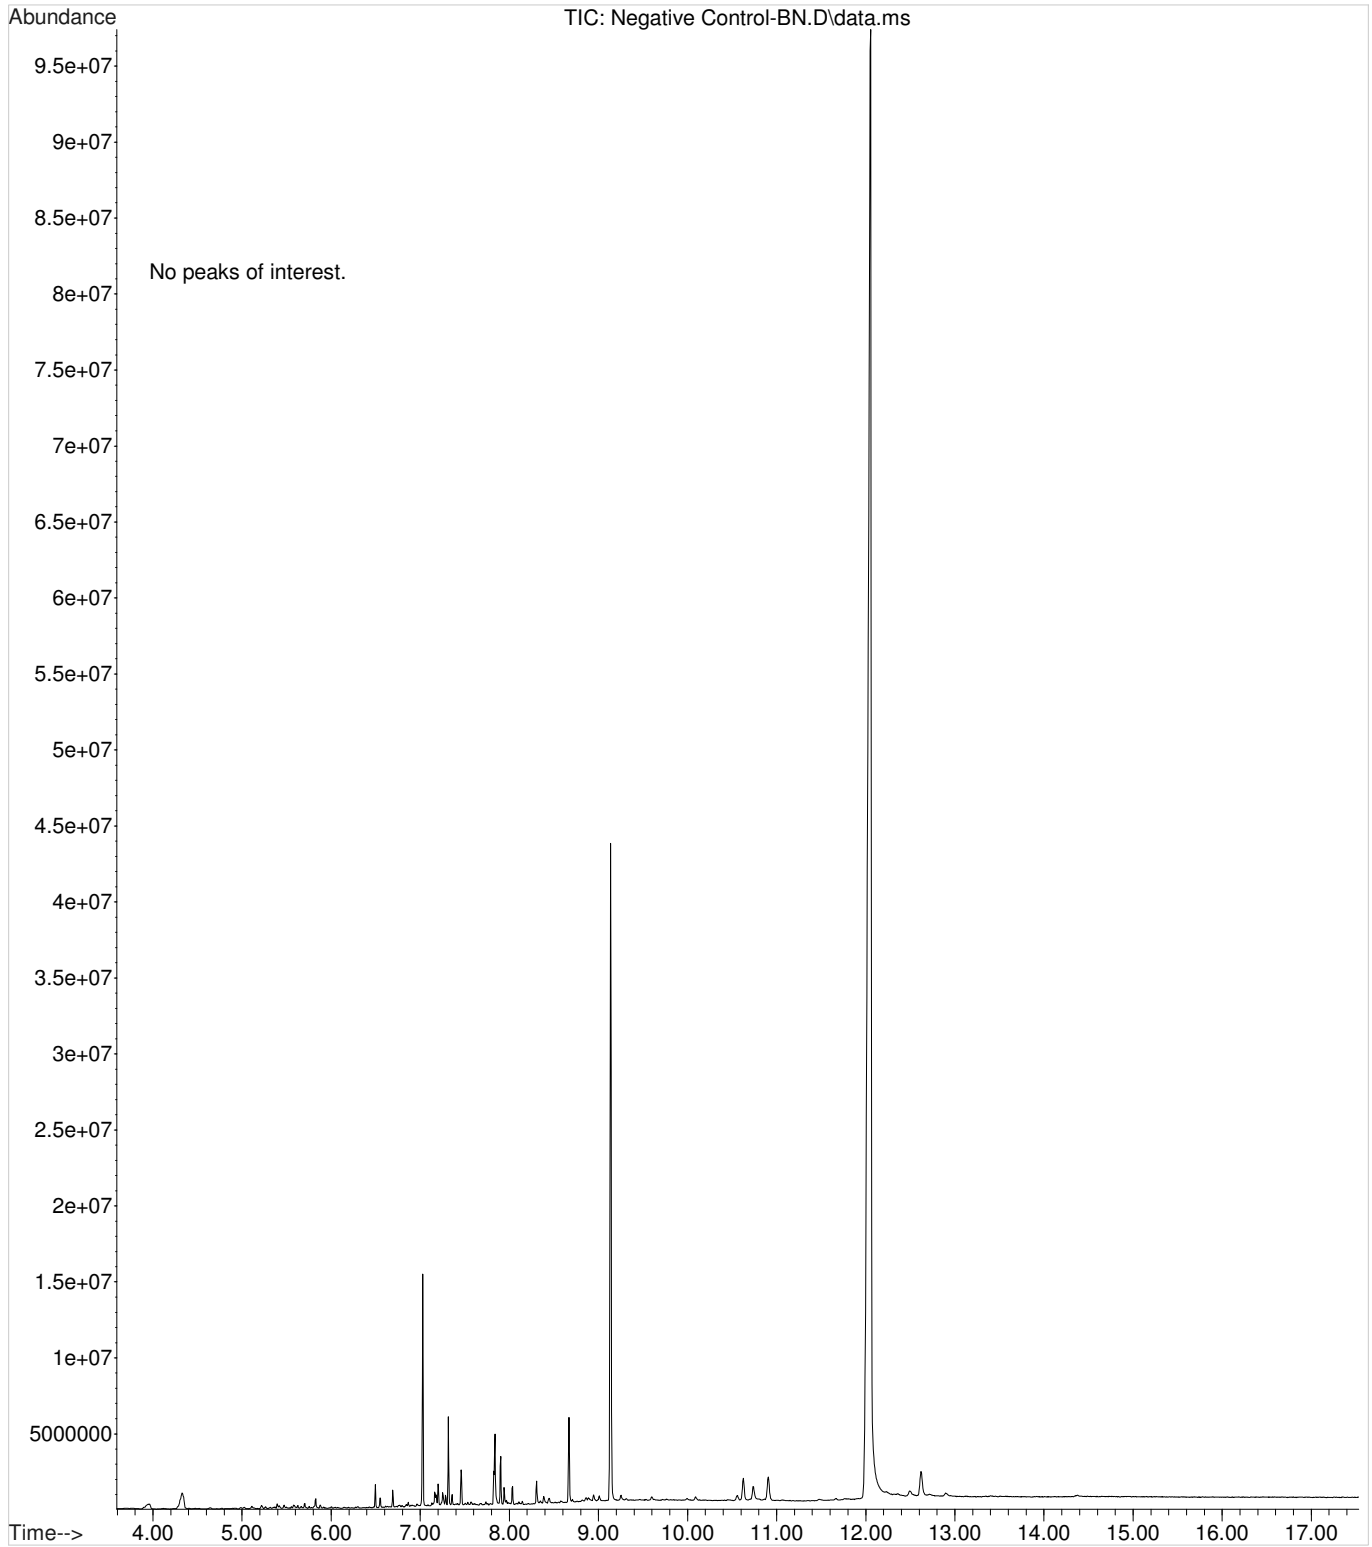


File :C:\MyFiles\cshrum\Desktop\101515 Data\Negative Control-BN.D
Operator : ISP\datastor
Acquired : 15 Oct 2015 19:55 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1
Vial Number: 1

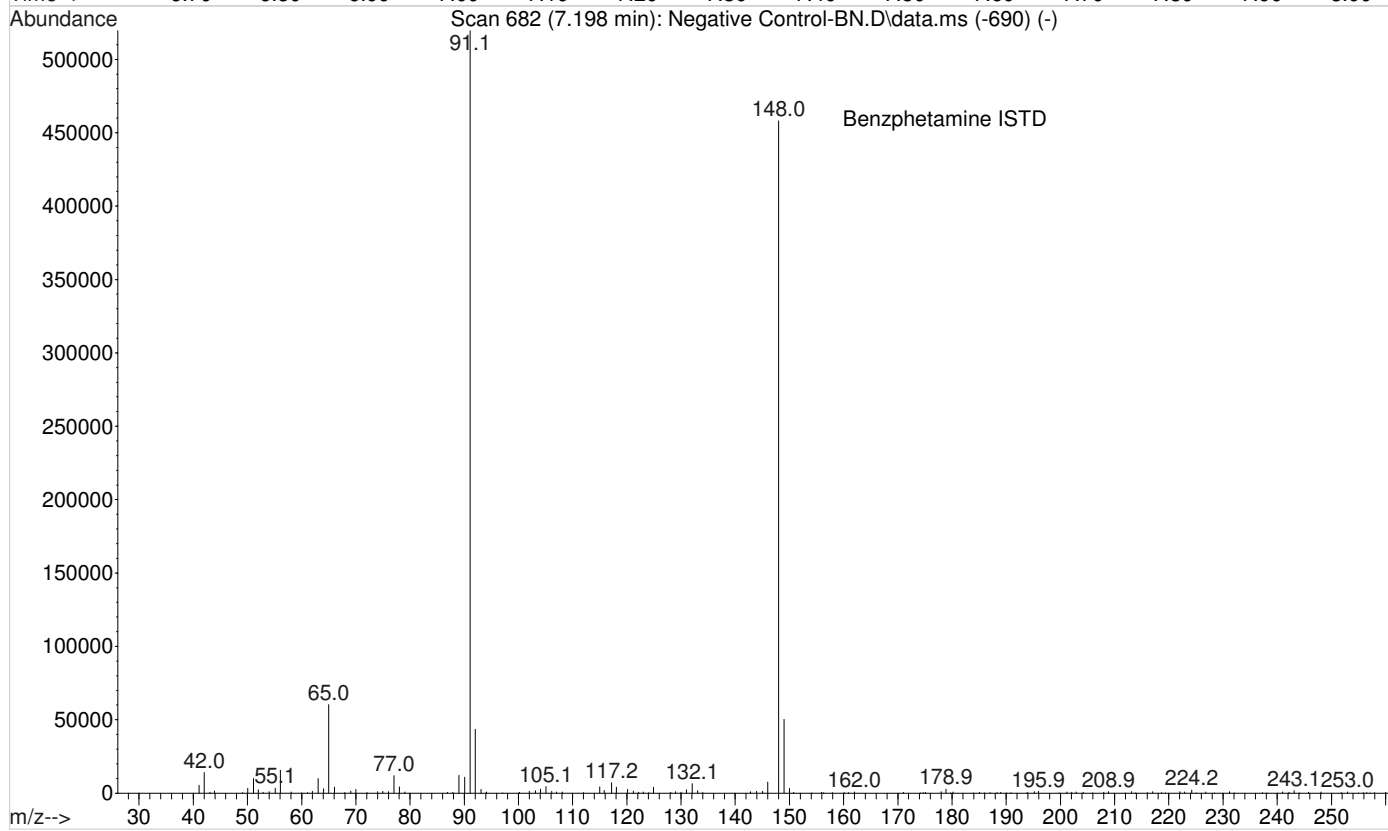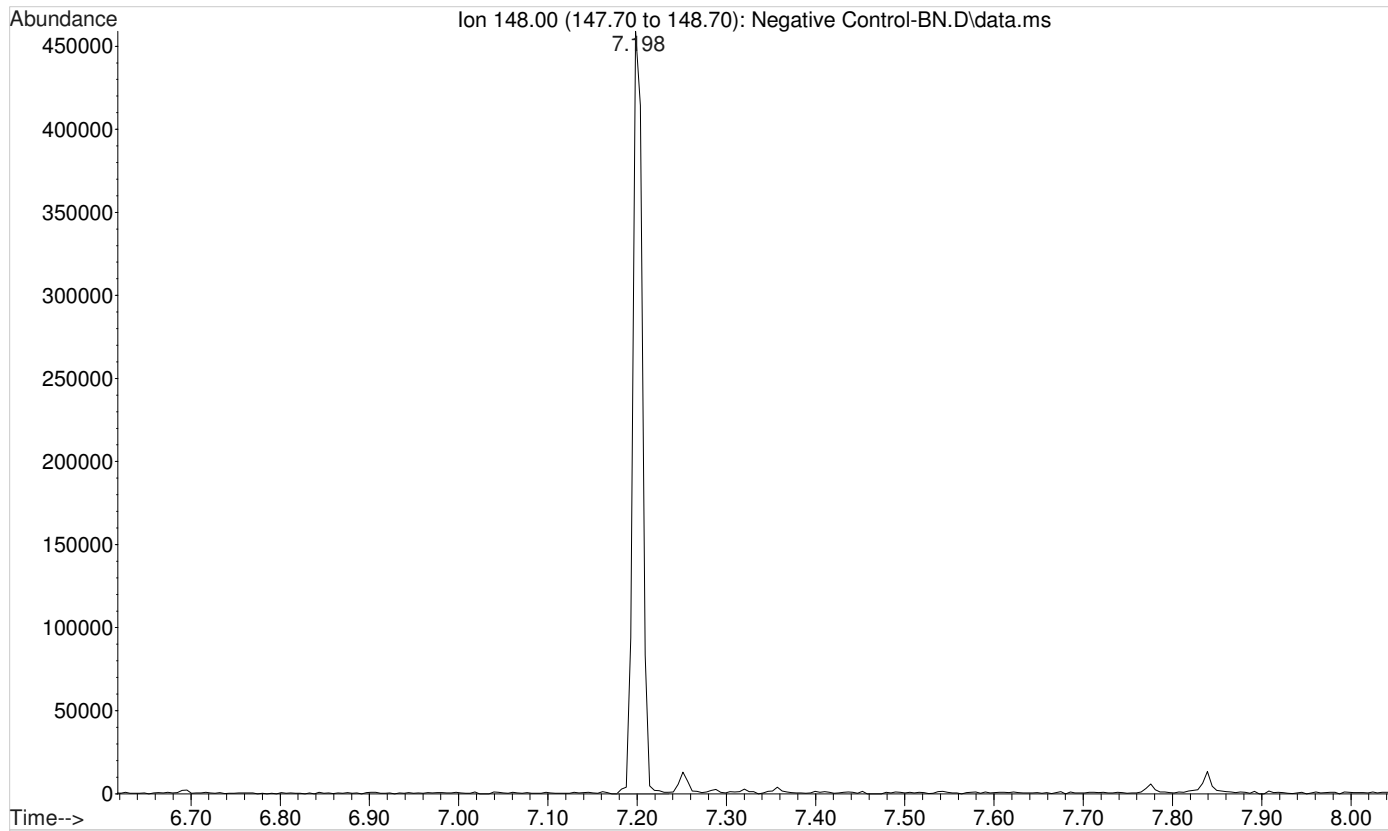



File :C:\MyFiles\cshrum\Desktop\101515 Data\Negative Control-BN.D
Operator : ISP\datastor
Acquired : 15 Oct 2015 19:55 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1
Vial Number: 1

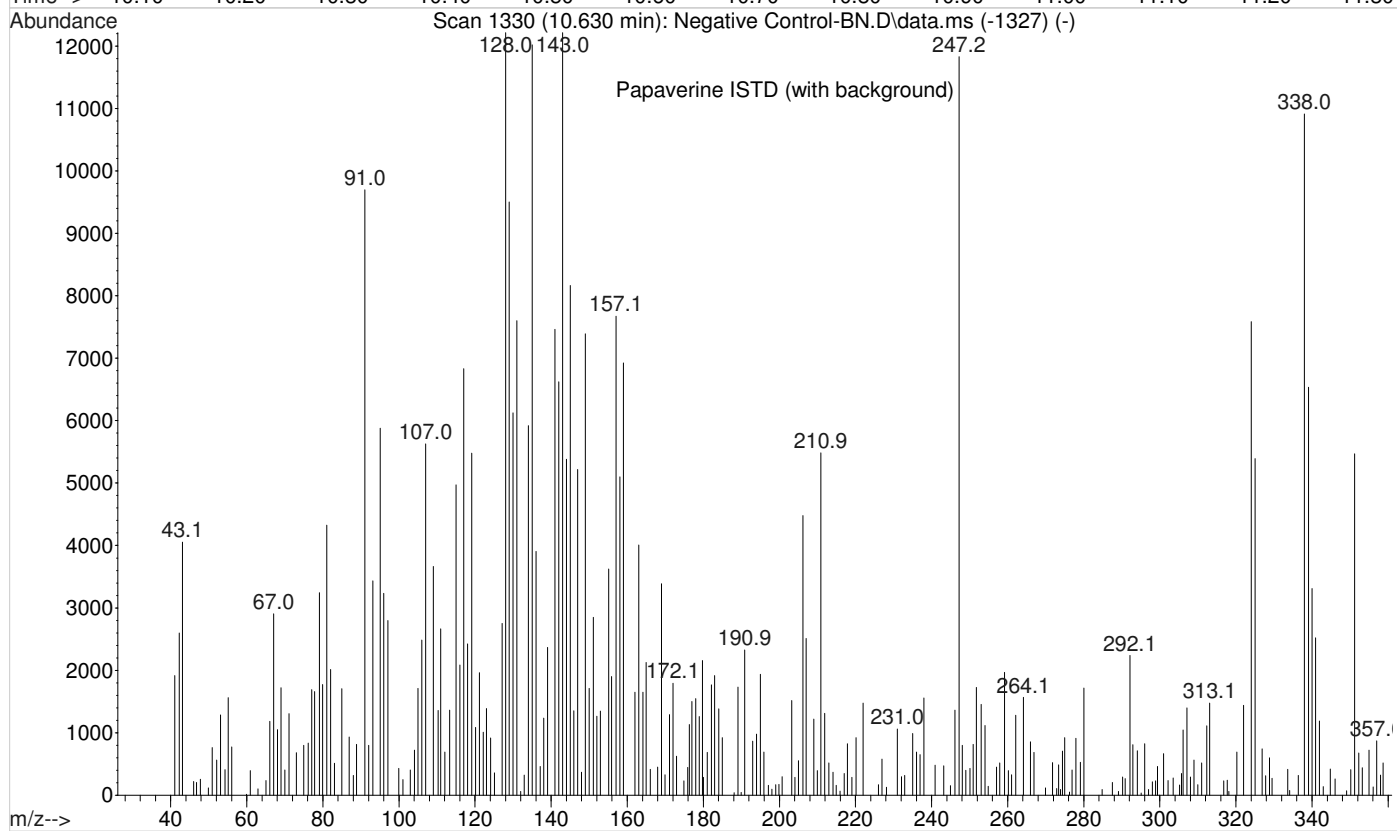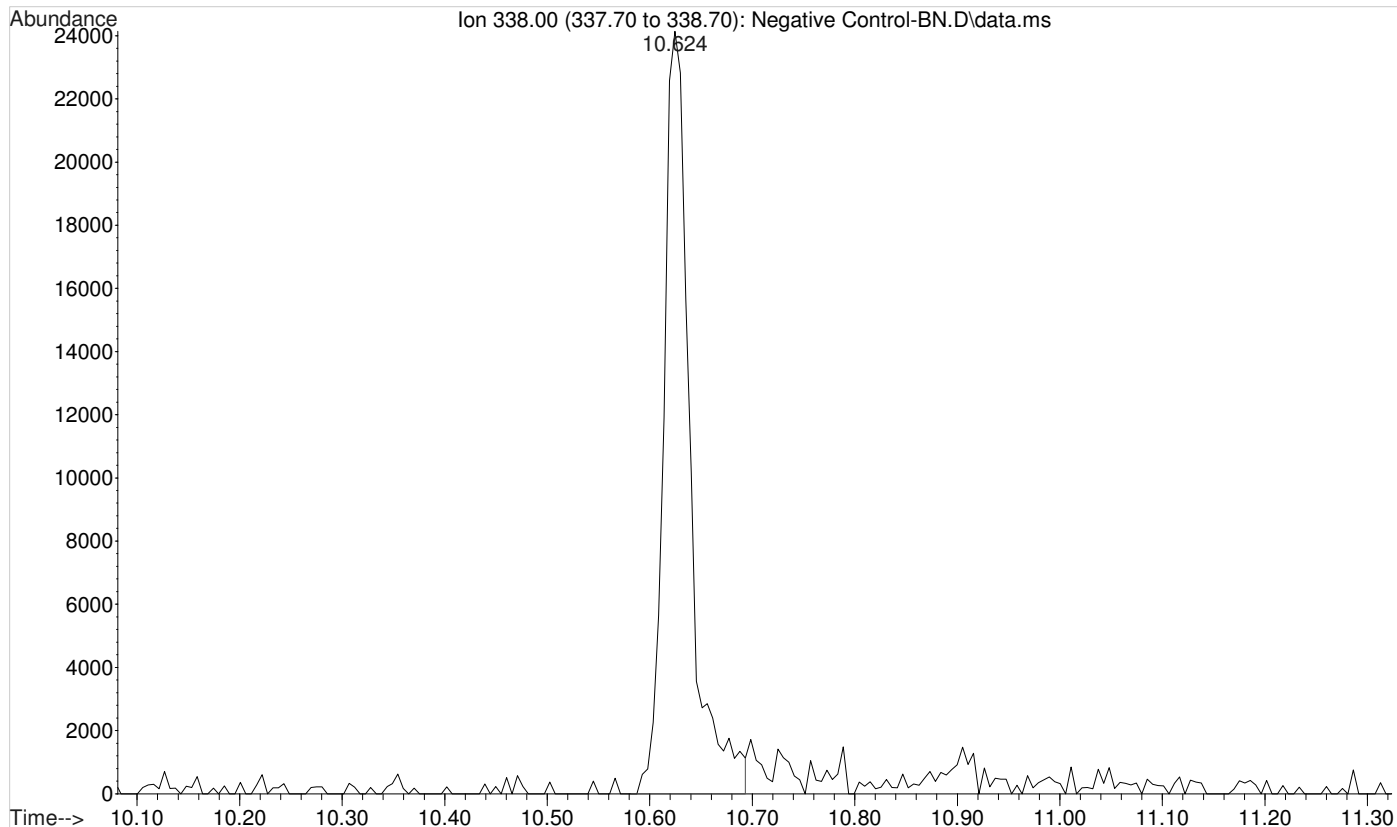



File :C:\MyFiles\cshrum\Desktop\101515 Data\Spiked Positive Contro
... 1-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 15 Oct 2015 20:18 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

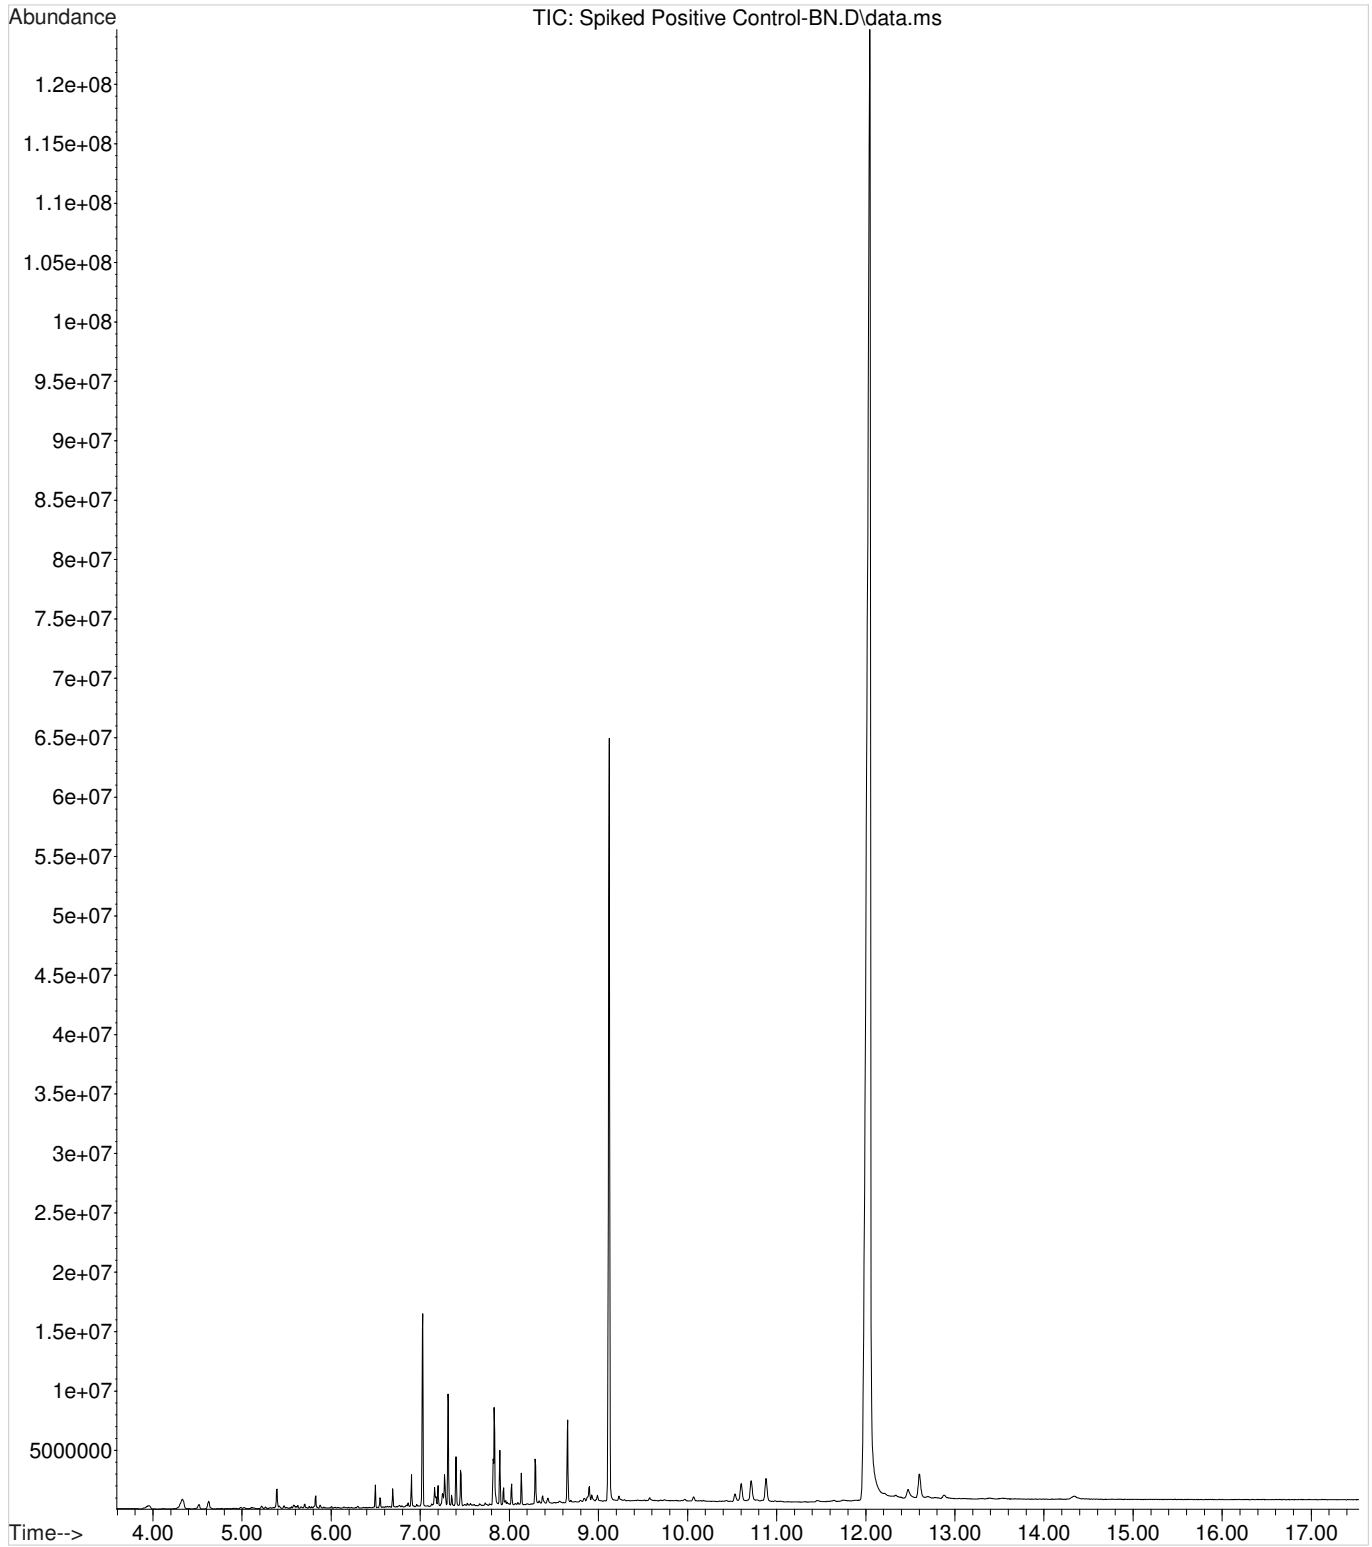



File :C:\MyFiles\cshrum\Desktop\101515 Data\Spiked Positive Contro
... l-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 15 Oct 2015 20:18 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

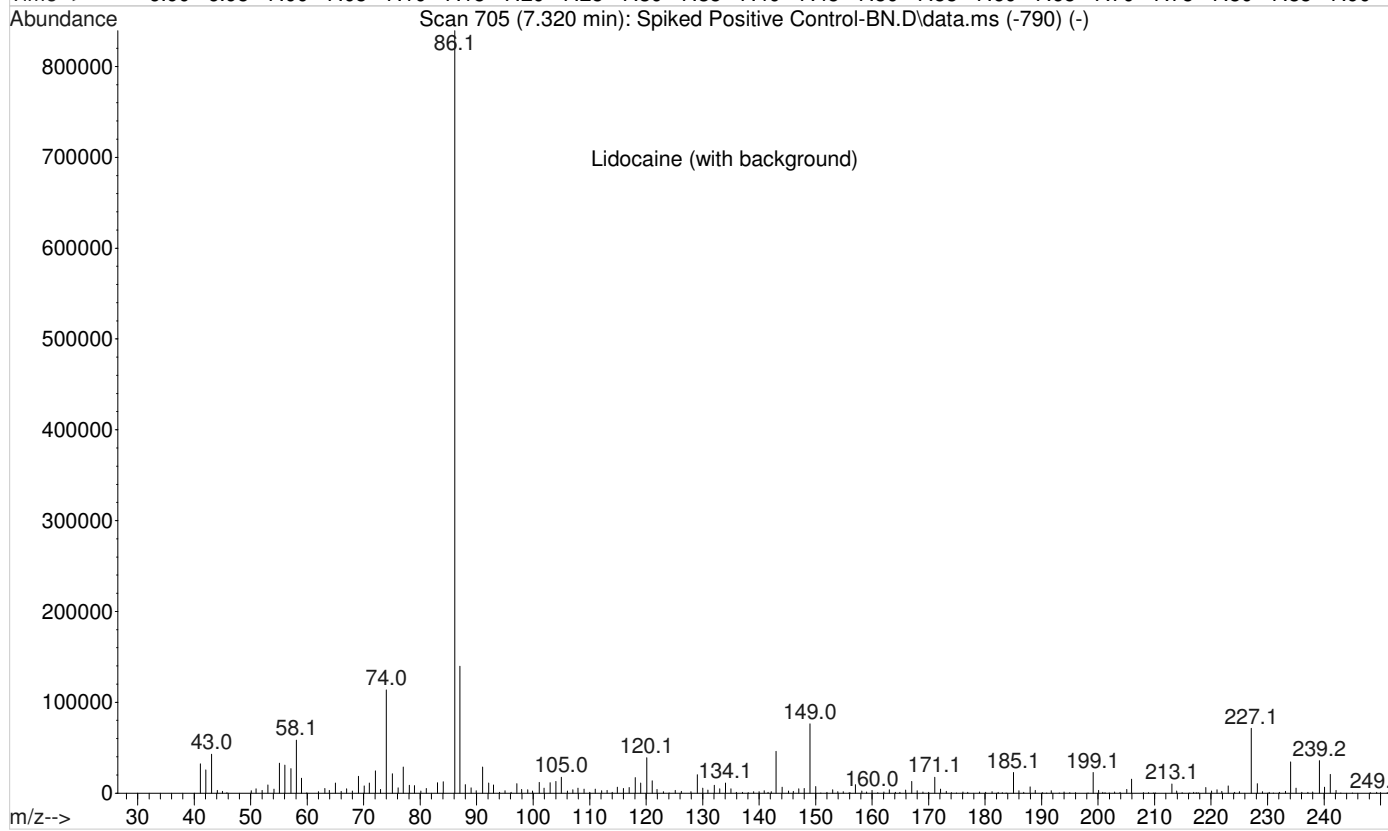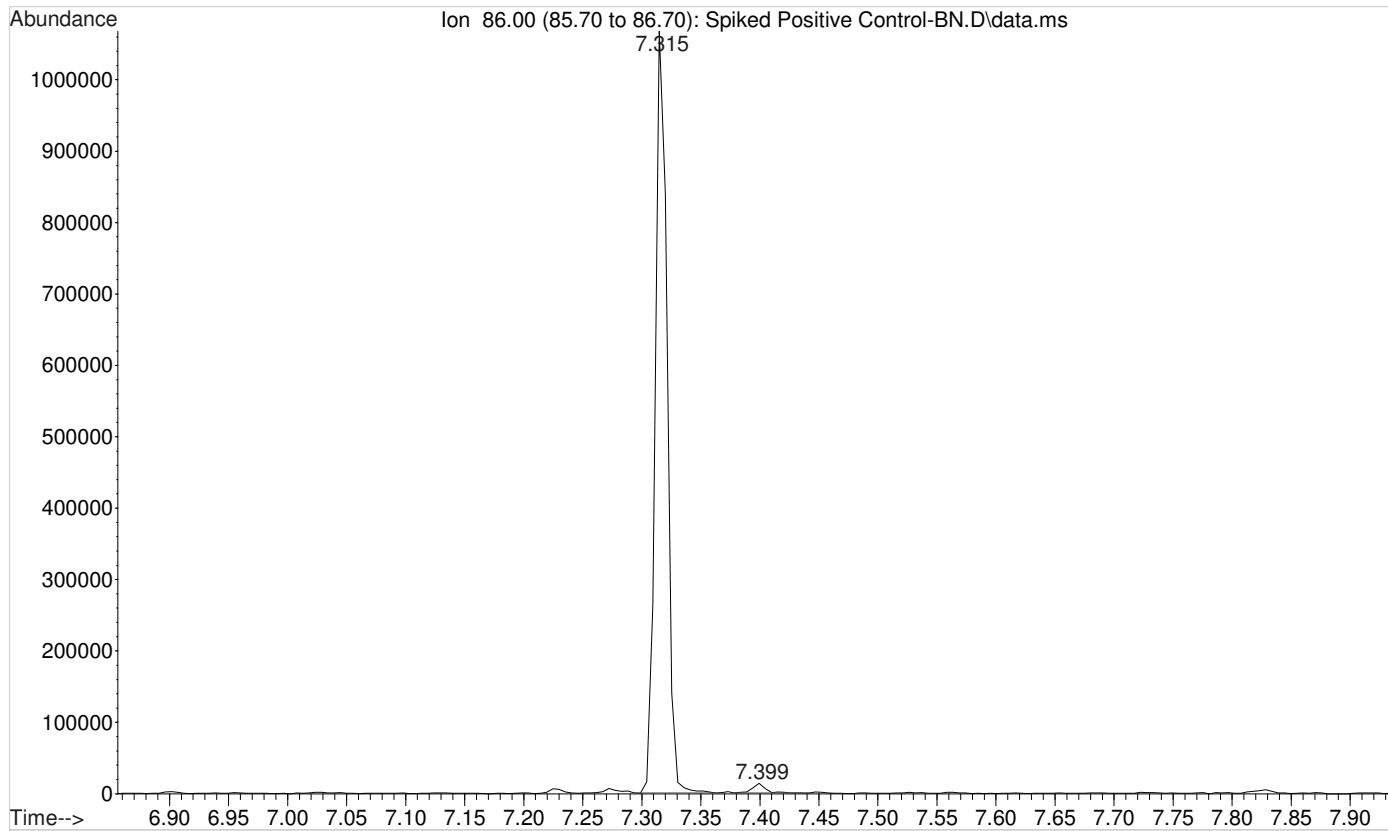



File :C:\MyFiles\cshrum\Desktop\101515 Data\Spiked Positive Contro
... l-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 15 Oct 2015 20:18 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

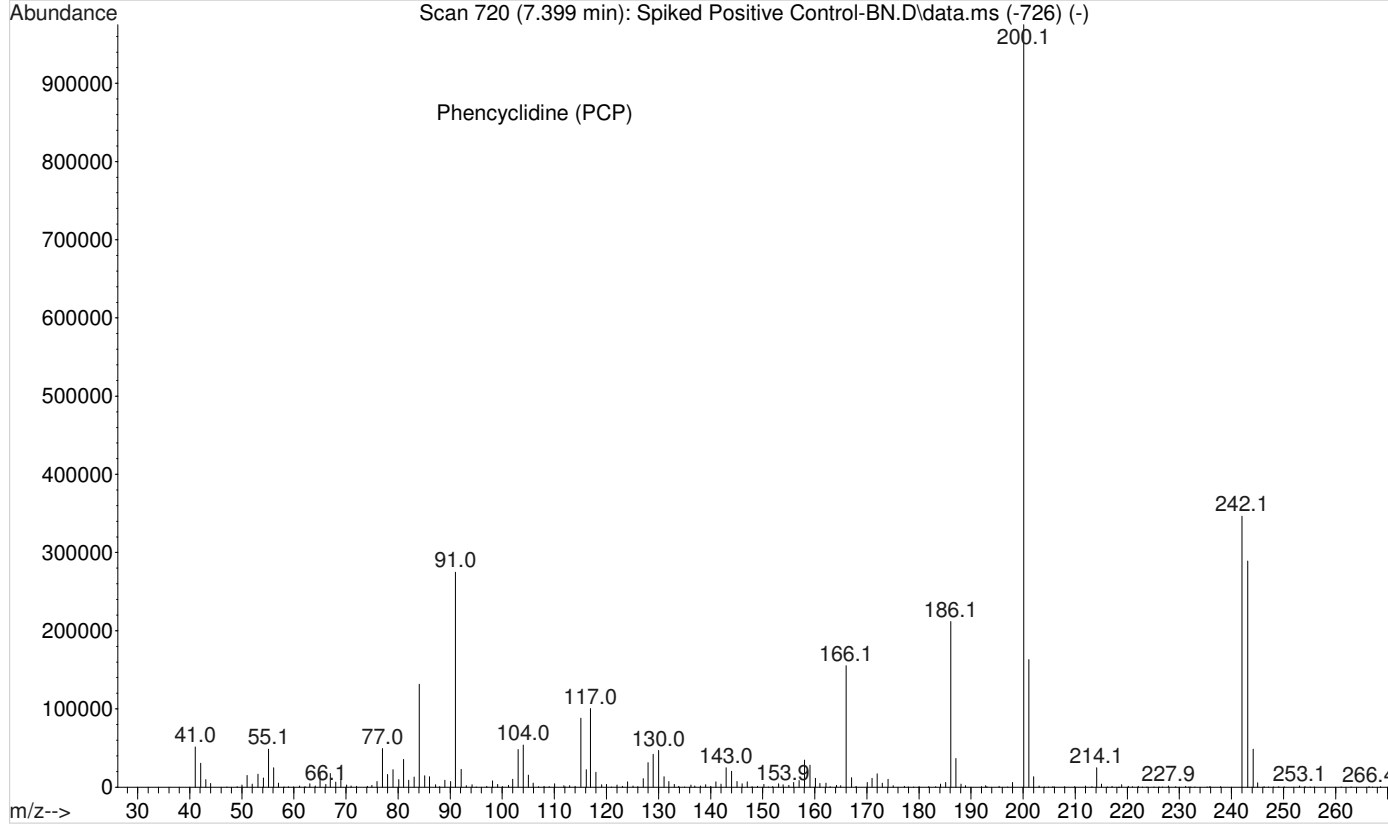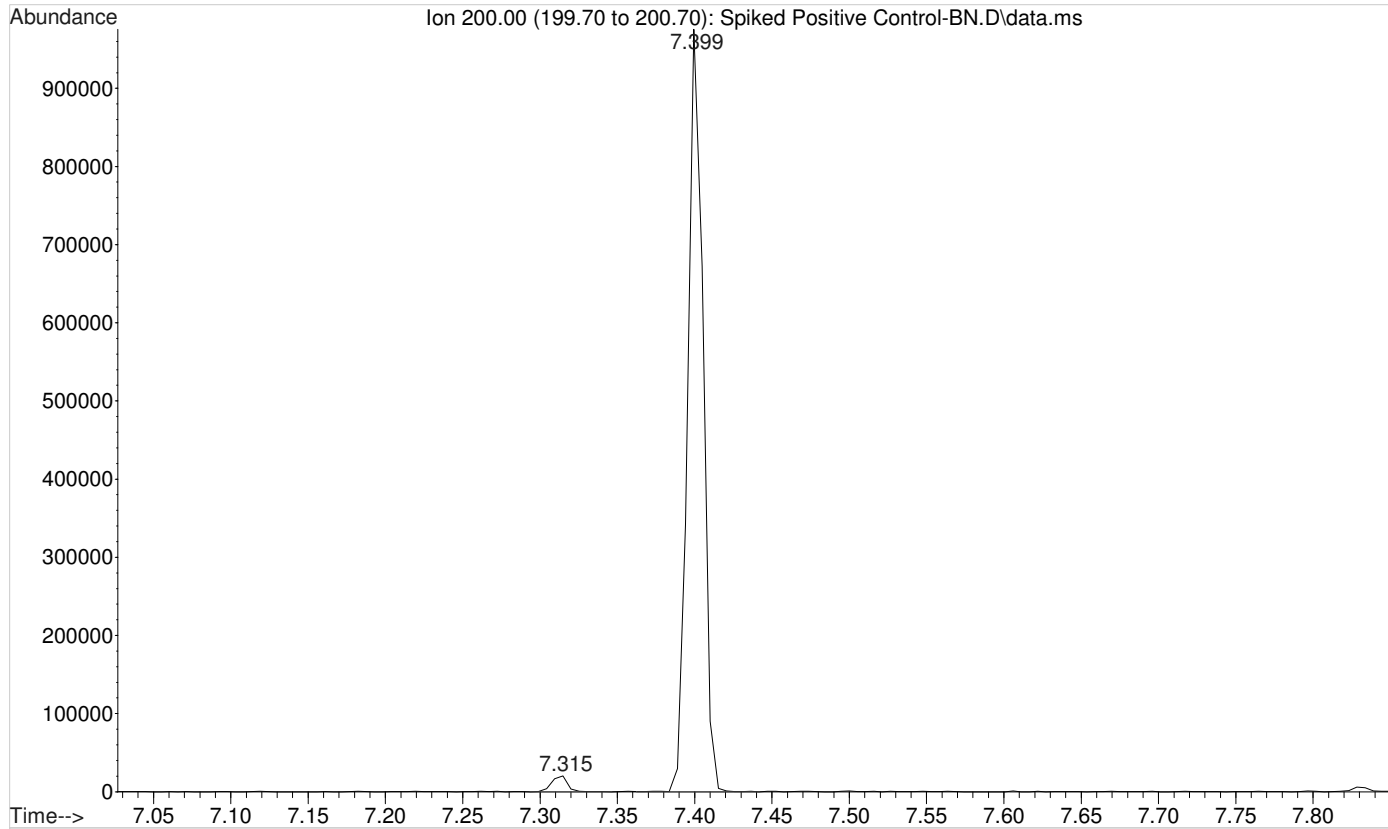



File :C:\MyFiles\cshrum\Desktop\101515 Data\Spiked Positive Contro
... l-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 15 Oct 2015 20:18 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

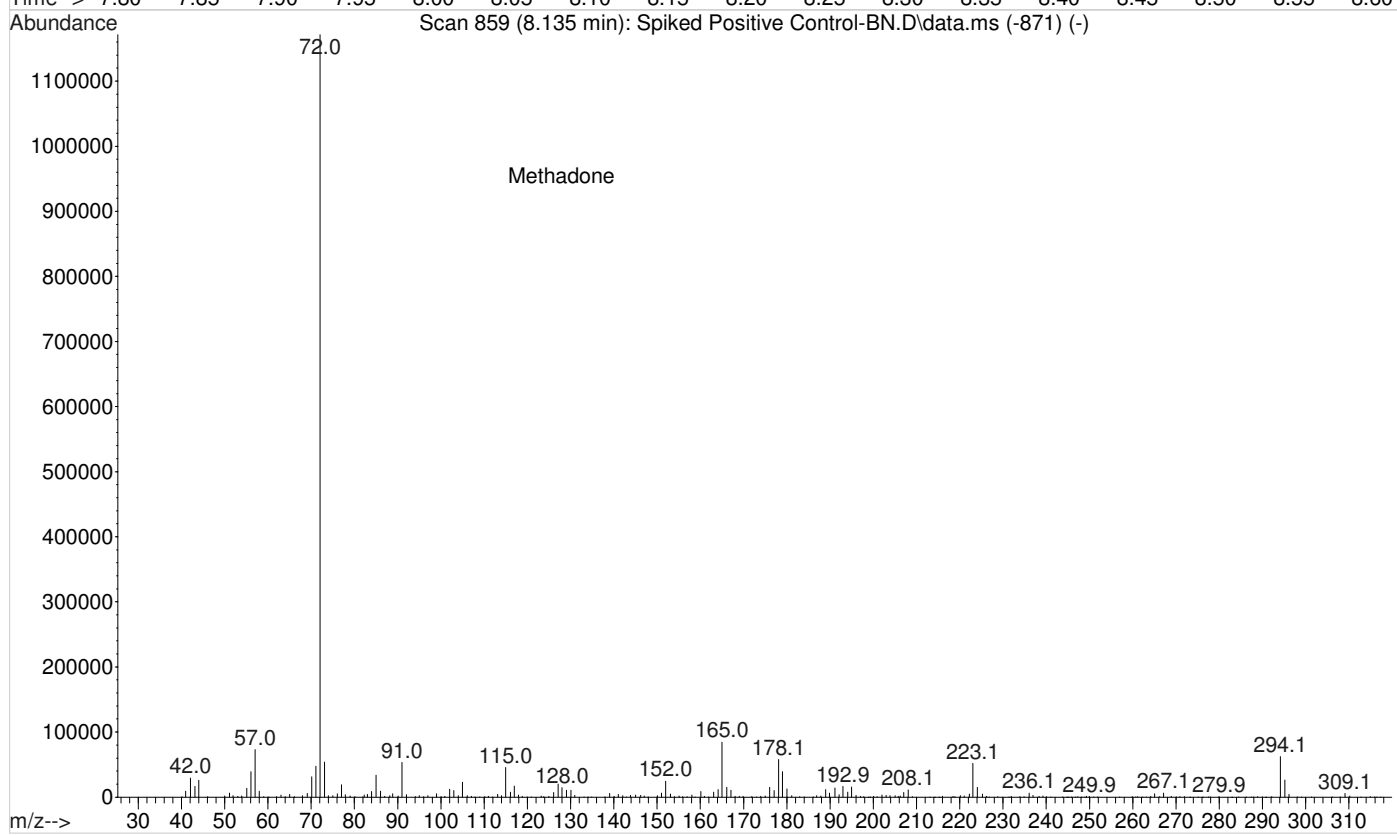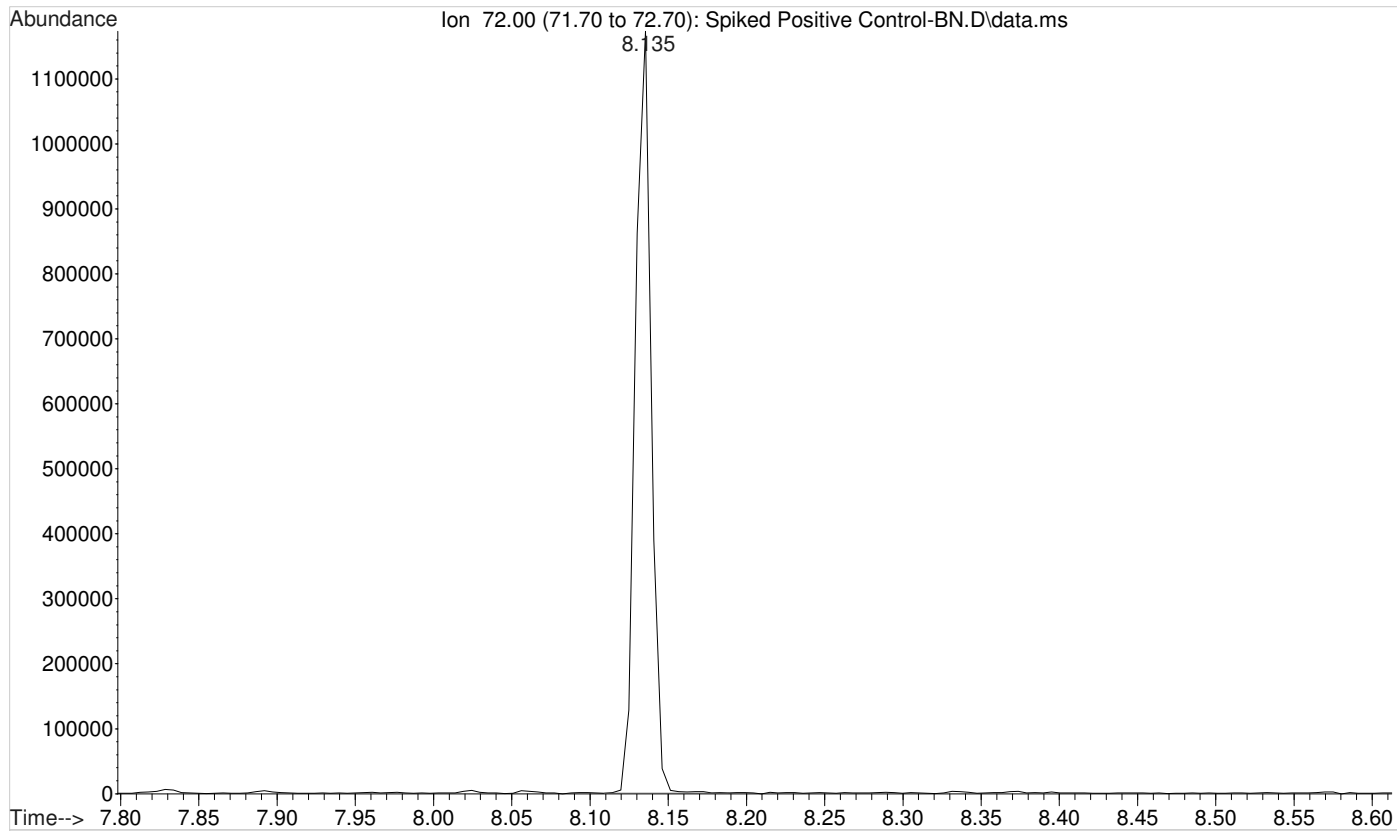



File :C:\MyFiles\cshrum\Desktop\101515 Data\Spiked Positive Contro
... l-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 15 Oct 2015 20:18 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

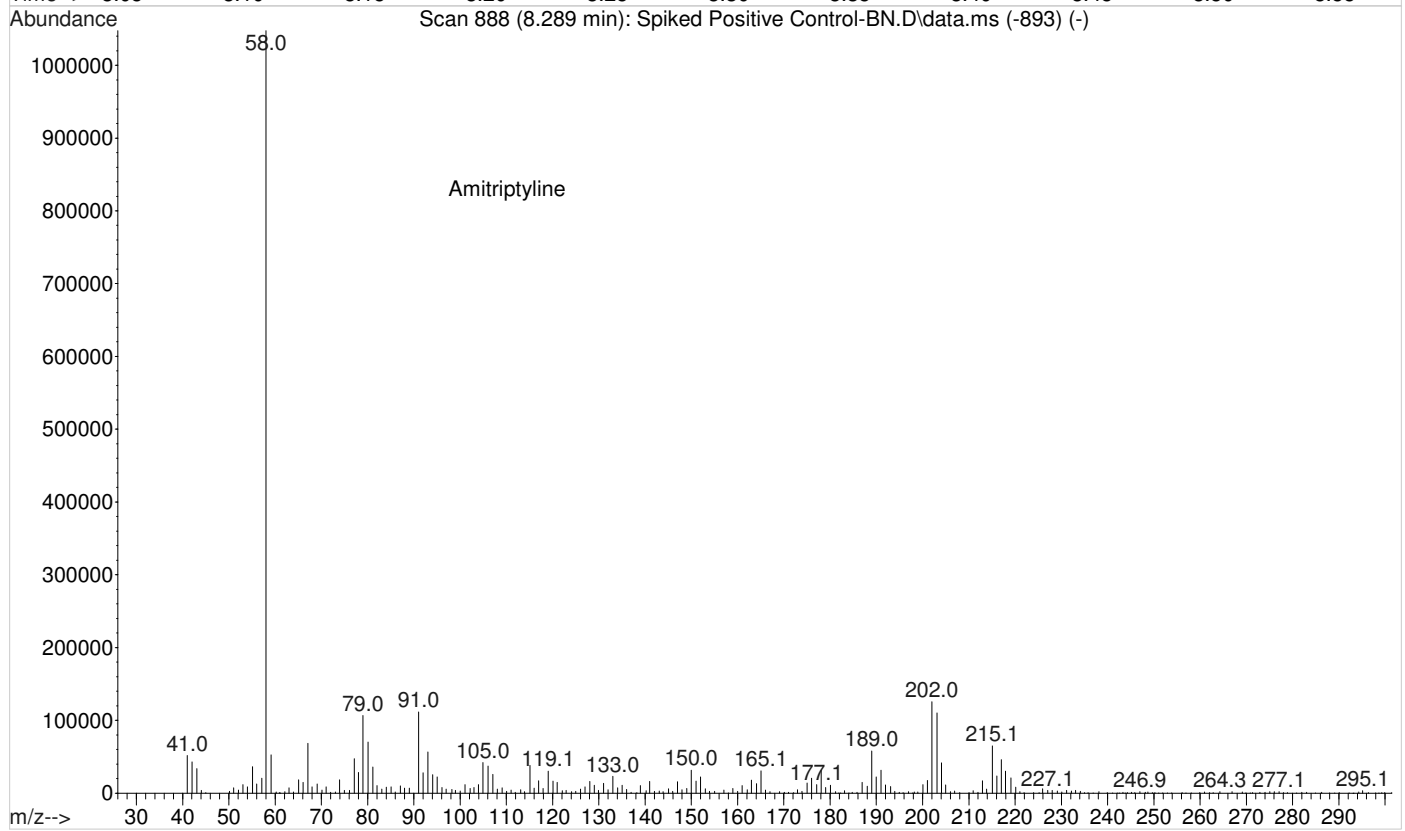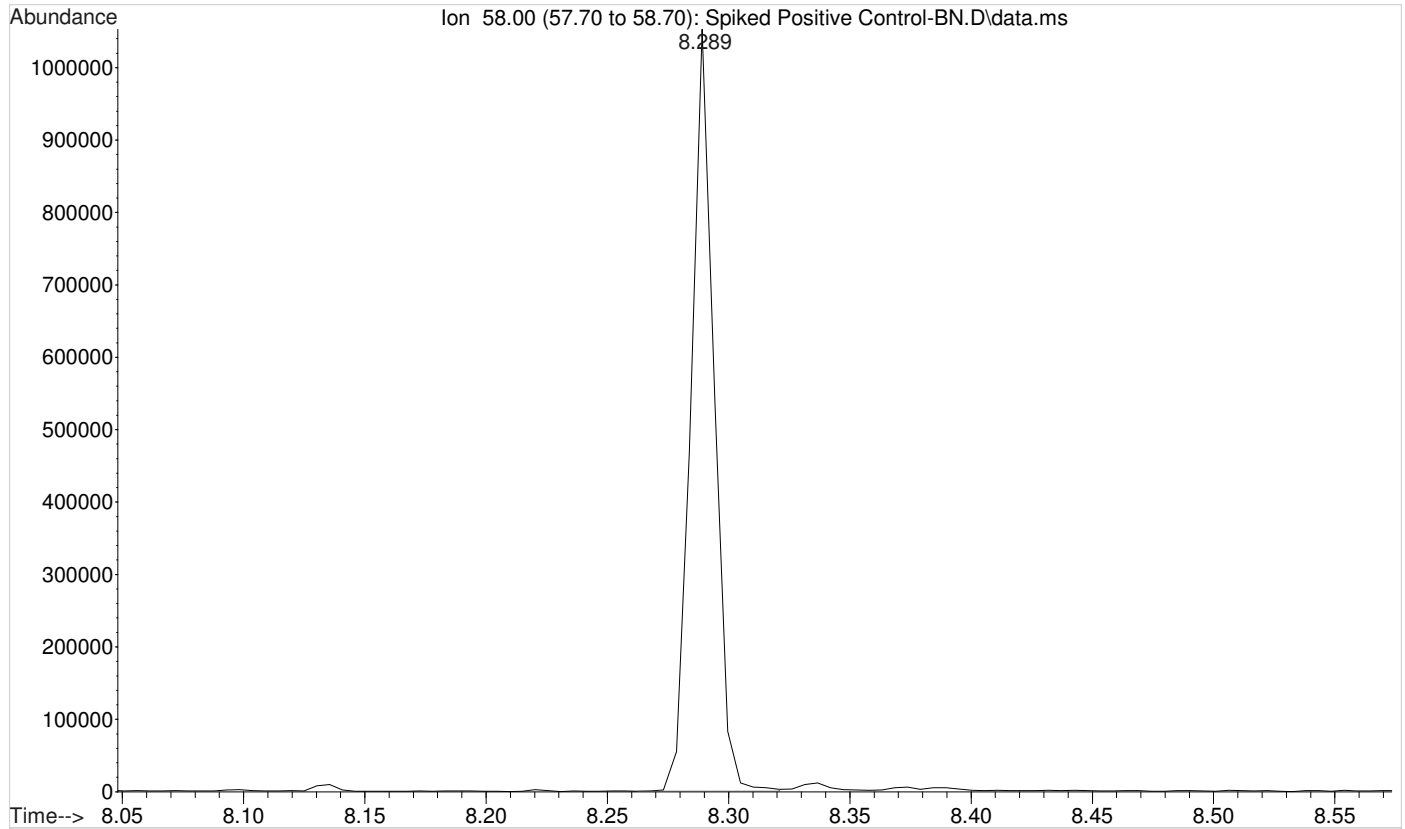



File :C:\MyFiles\cshrum\Desktop\101515 Data\Spiked Positive Contro
... l-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 15 Oct 2015 20:18 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

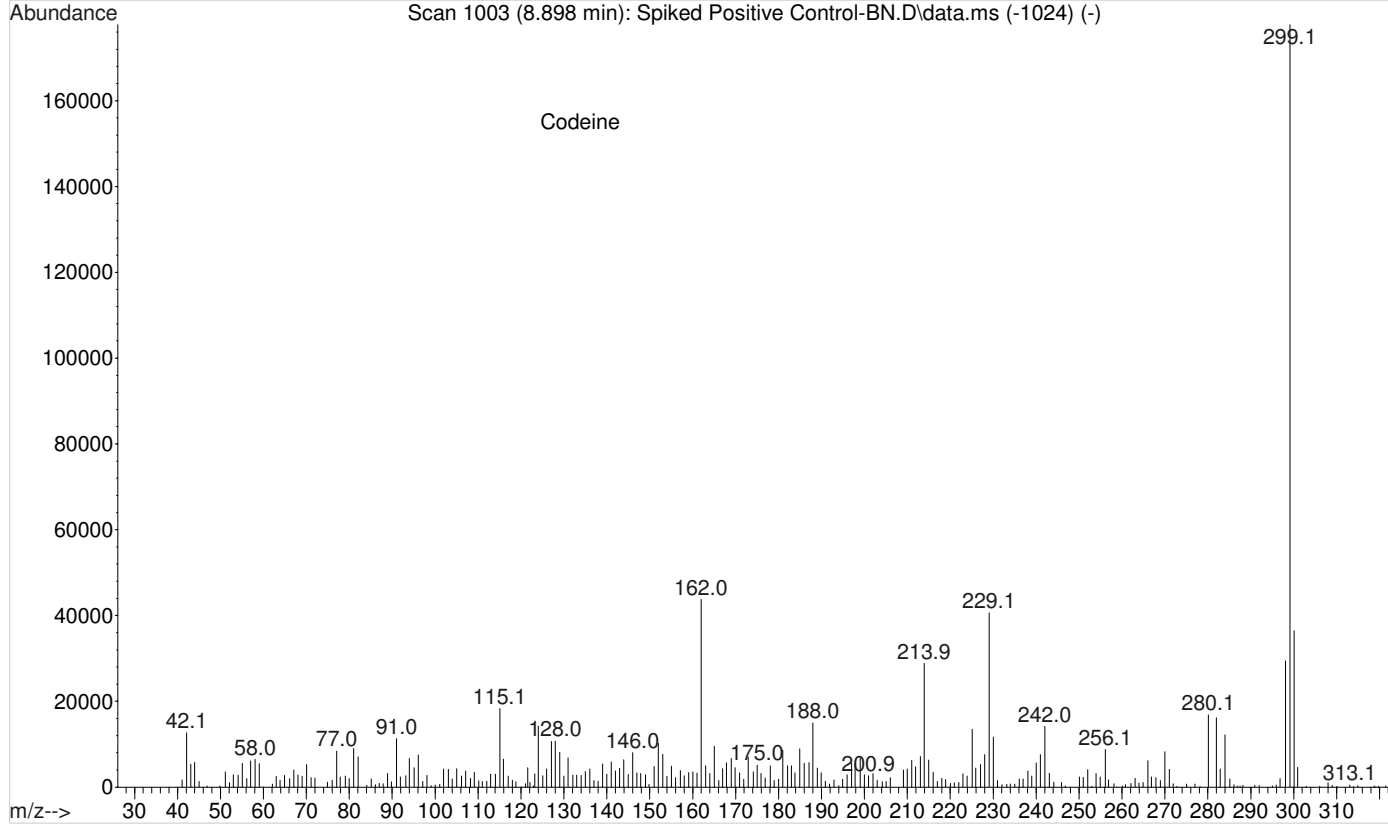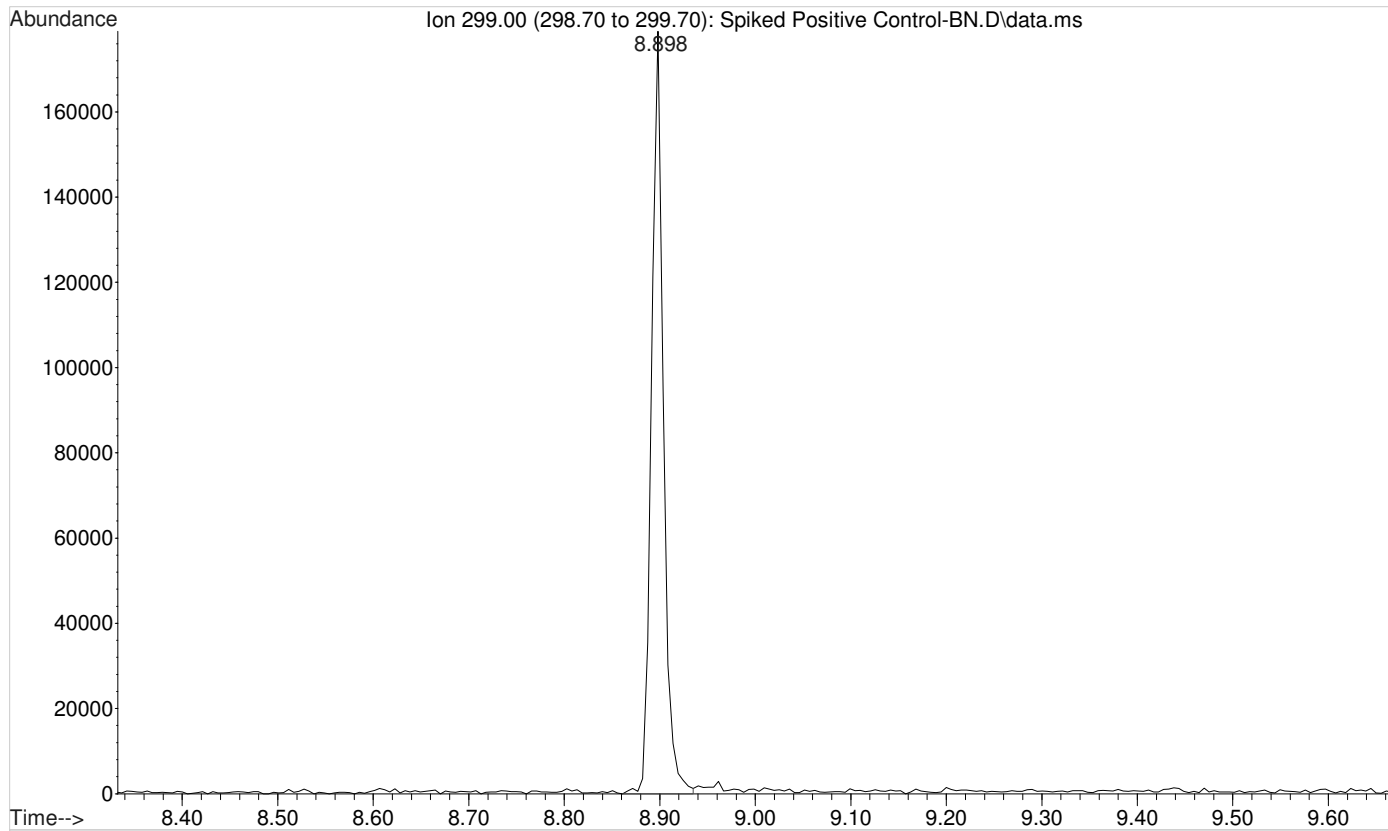



File :C:\MyFiles\cshrum\Desktop\101515 Data\Spiked Positive Contro
... l-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 15 Oct 2015 20:18 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

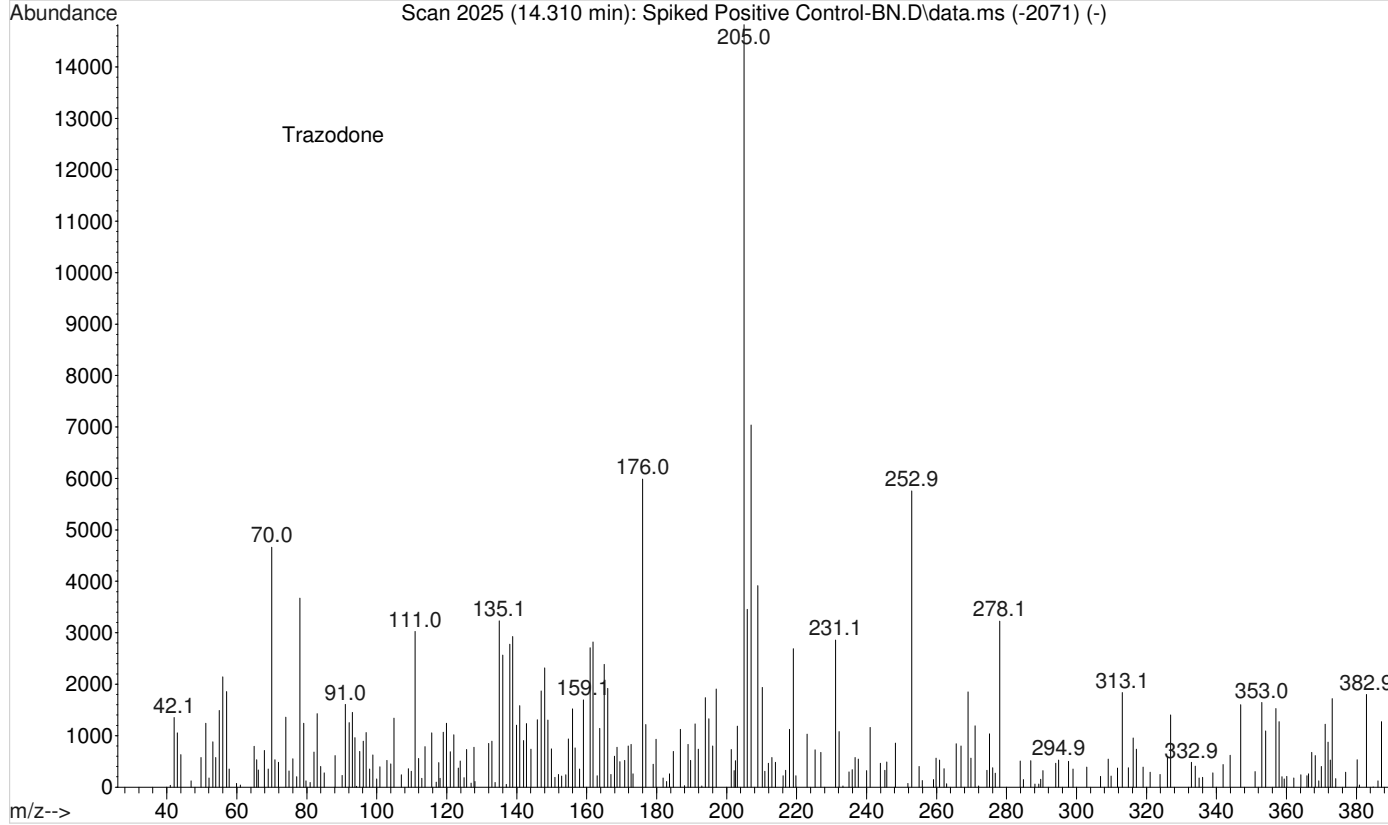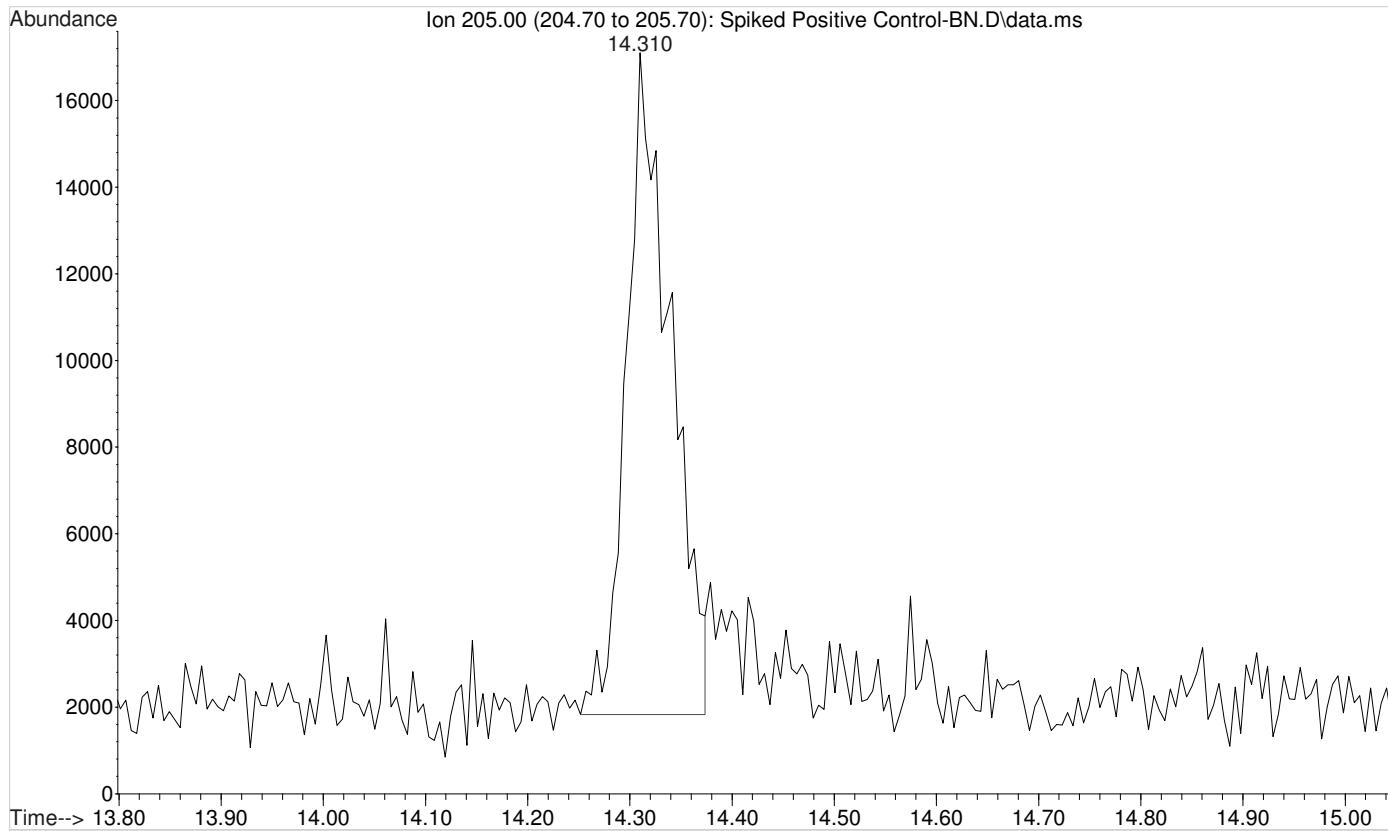



File :C:\MyFiles\cshrum\Desktop\101515 Data\Spiked Positive Contro
... l-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 15 Oct 2015 20:18 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

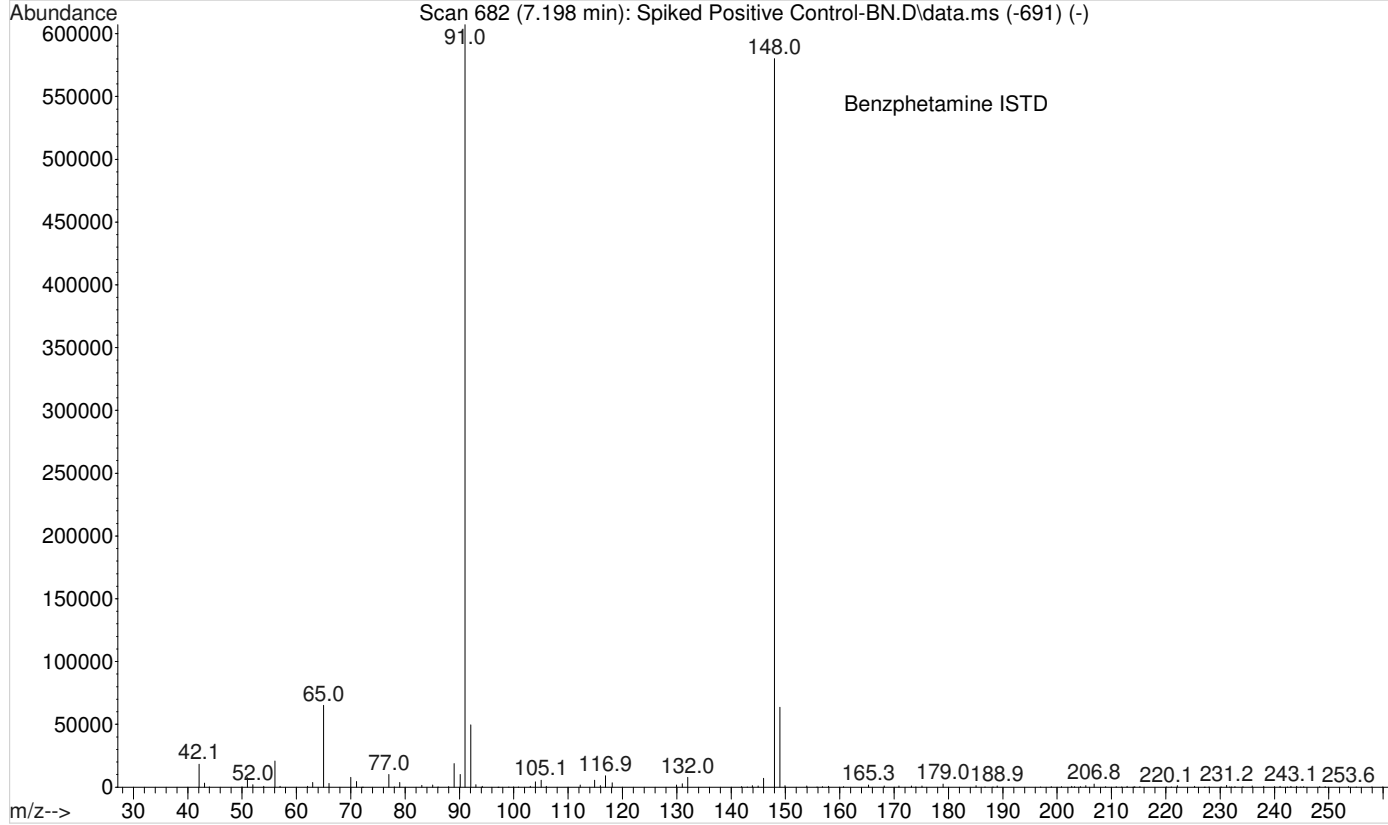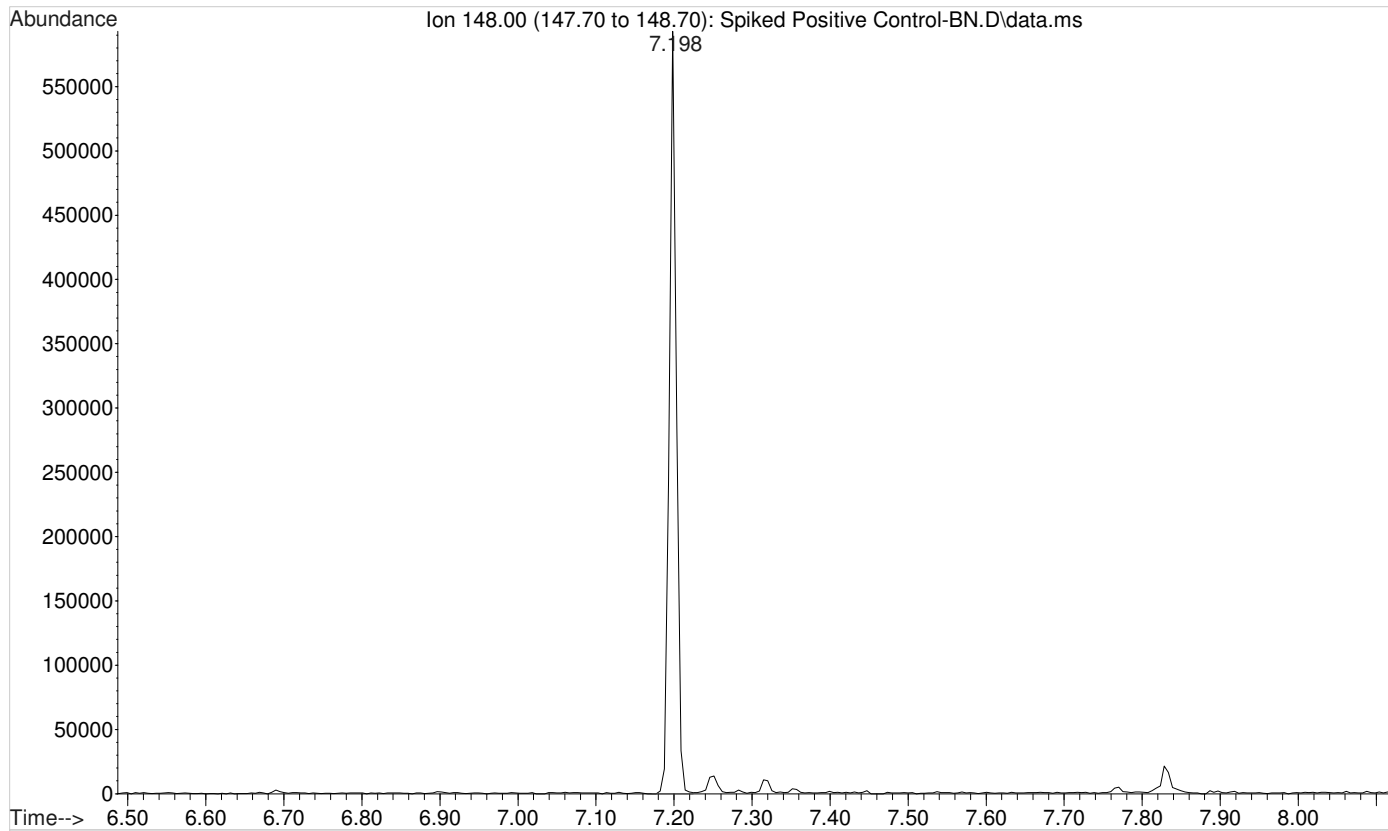



File :C:\MyFiles\cshrum\Desktop\101515 Data\Spiked Positive Contro
... l-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 15 Oct 2015 20:18 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

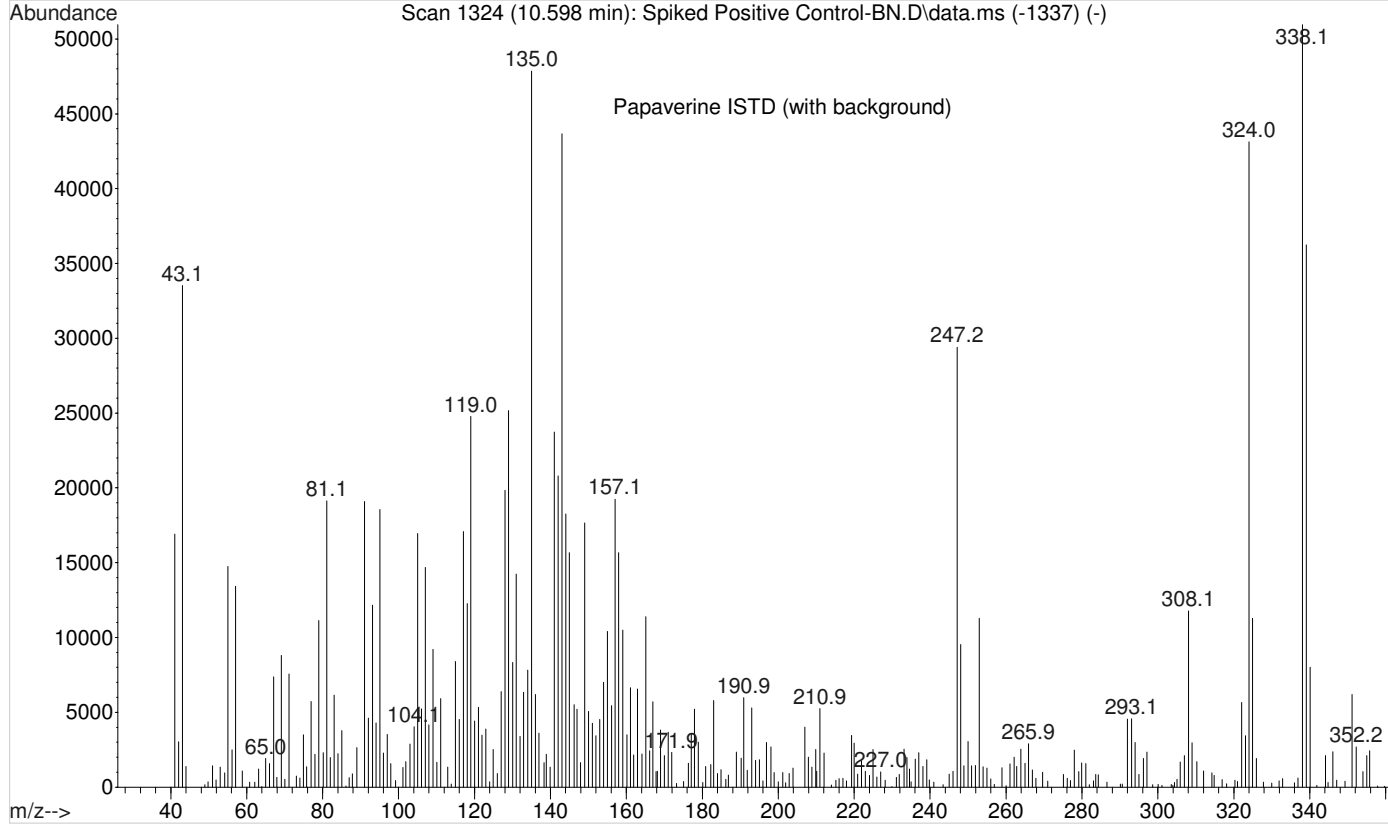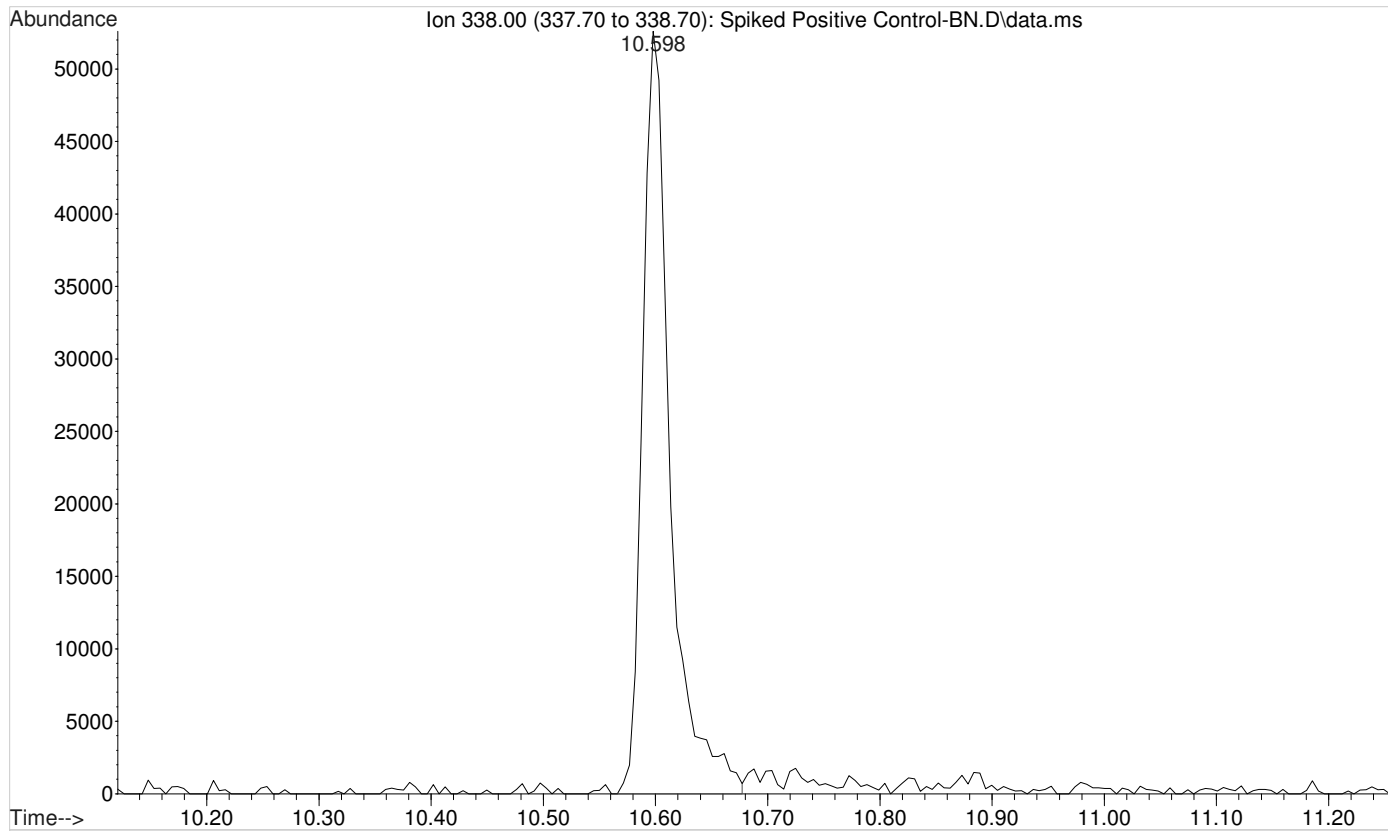



File :C:\MyFiles\cshrum\Desktop\101515 Data\Spiked Positive Contro
... l-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 15 Oct 2015 20:18 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

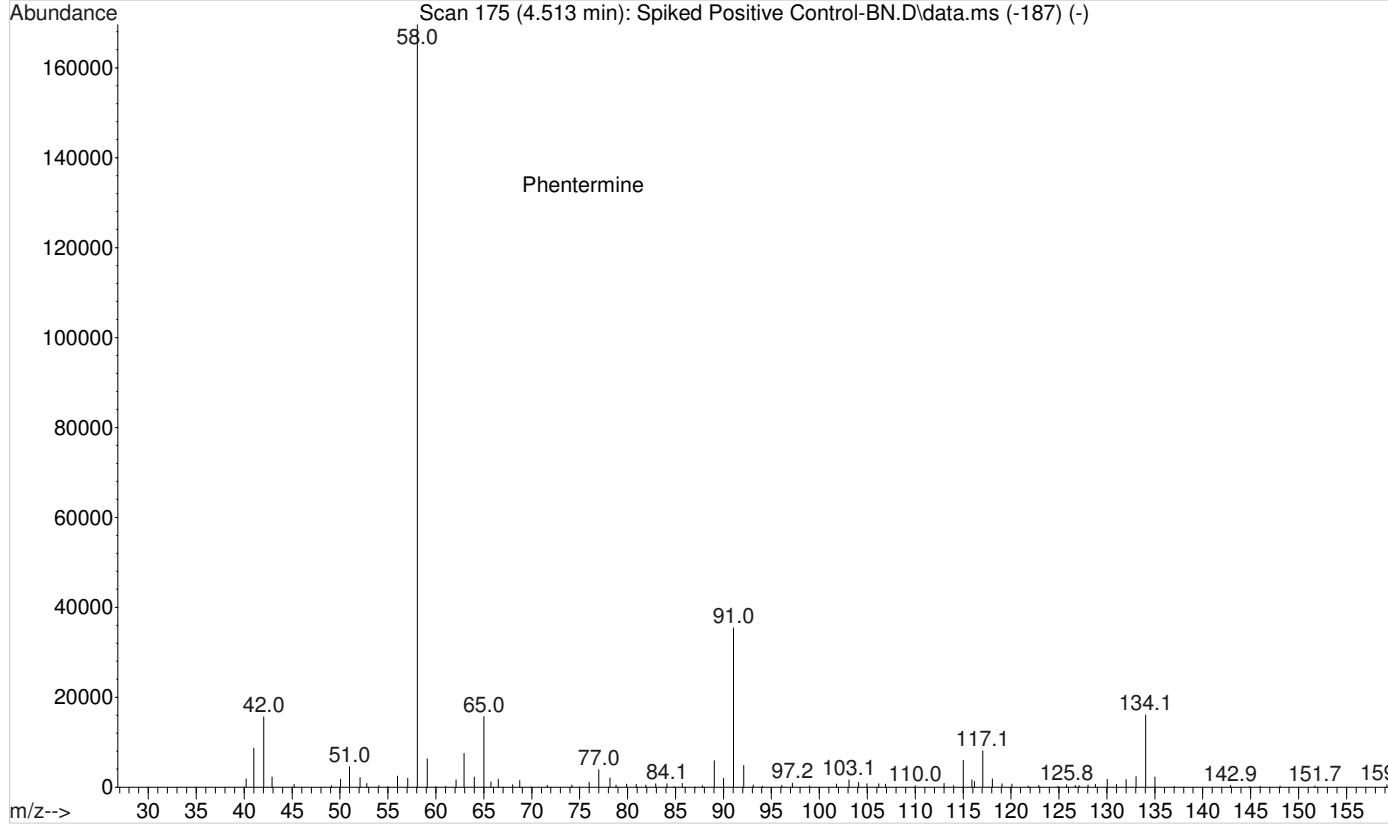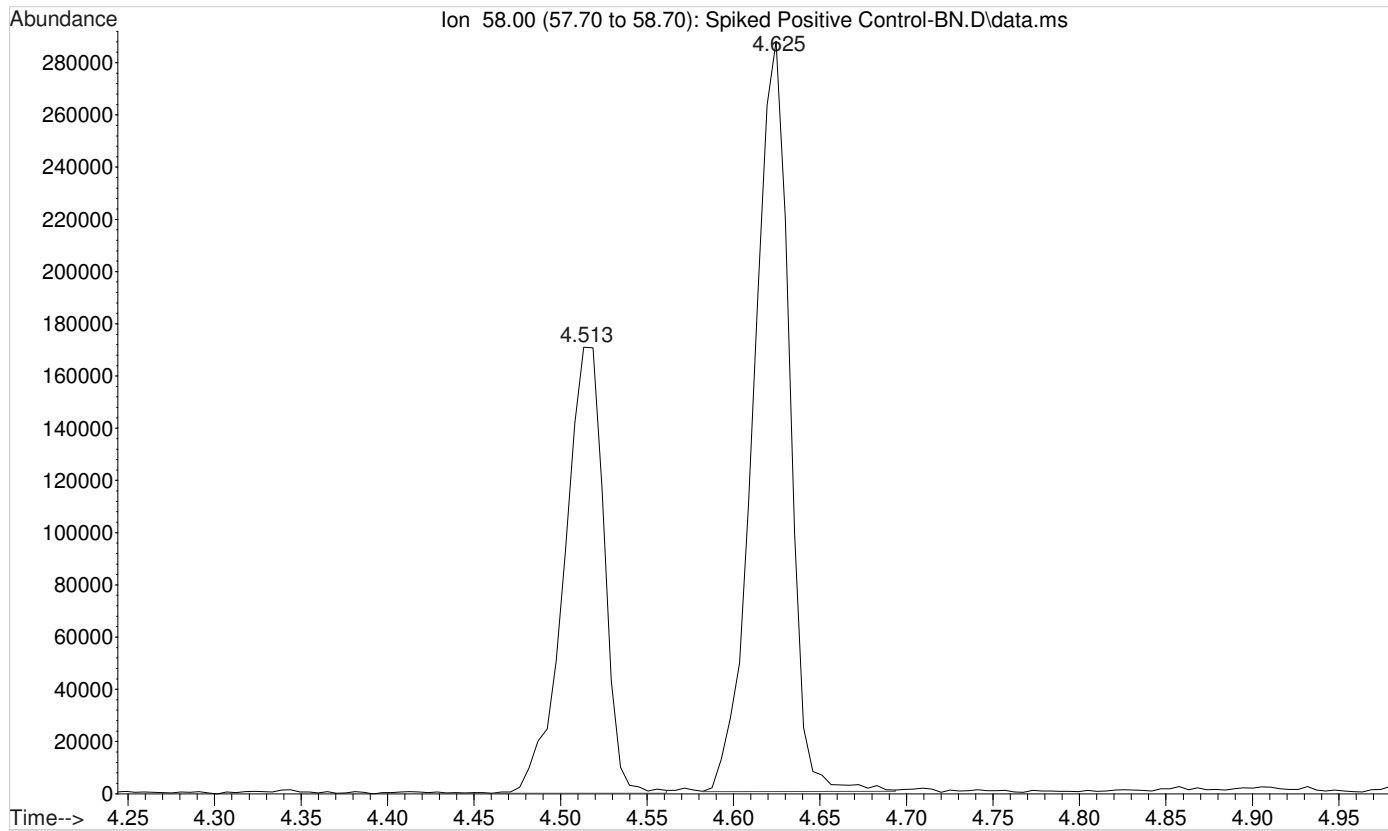



File :C:\MyFiles\cshrum\Desktop\101515 Data\Spiked Positive Control
... 1-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 15 Oct 2015 20:18 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

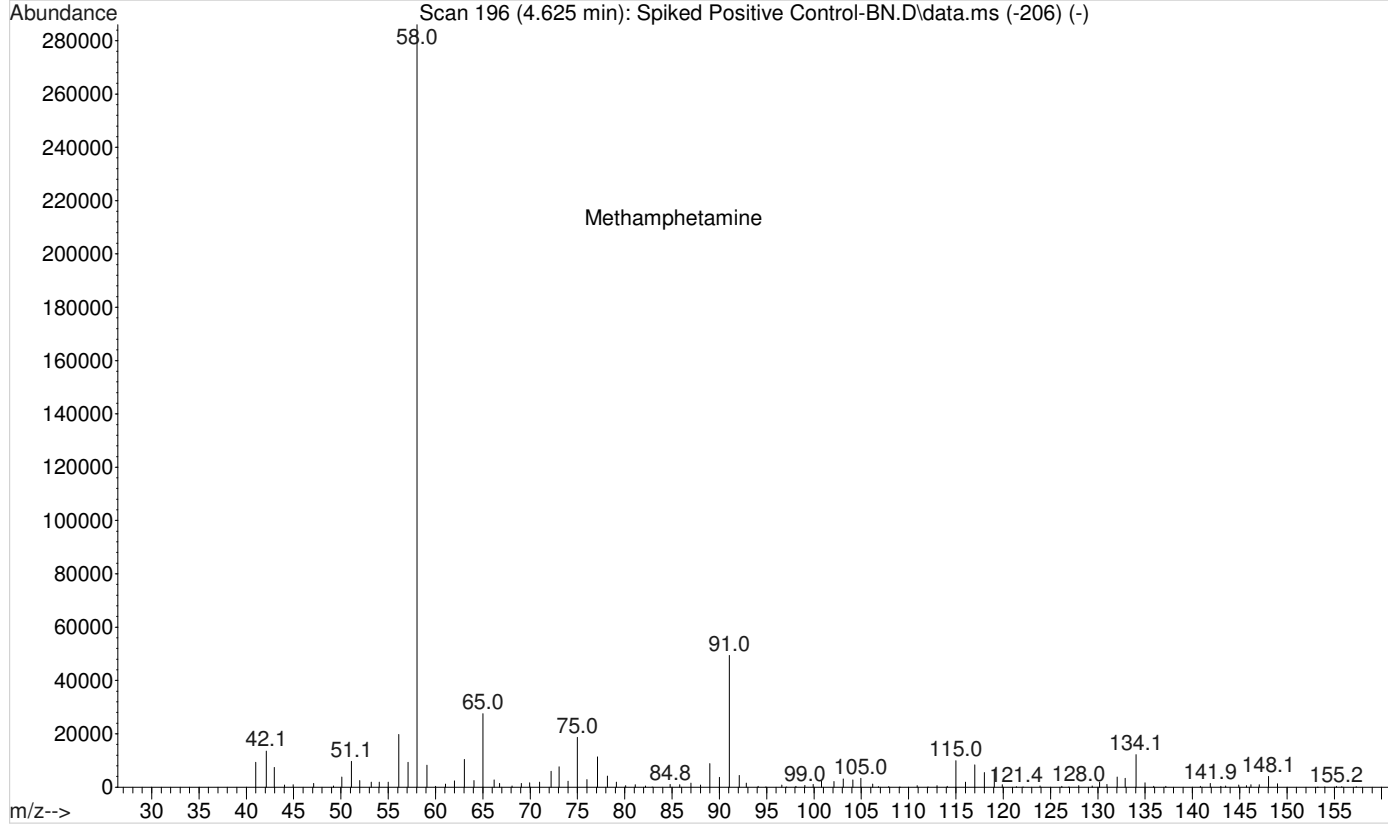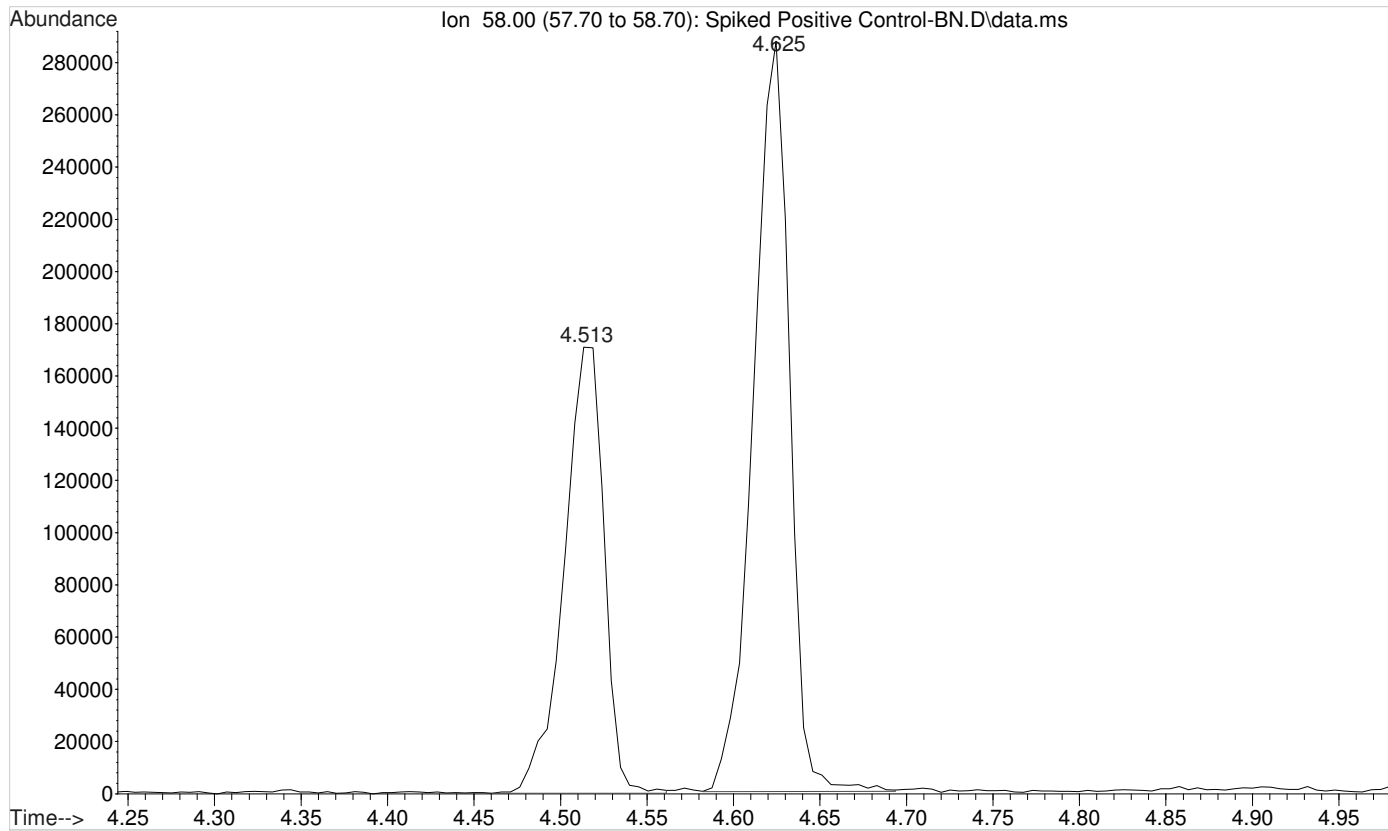



File :C:\MyFiles\cshrum\Desktop\101515 Data\Spiked Positive Contro
... l-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 15 Oct 2015 20:18 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

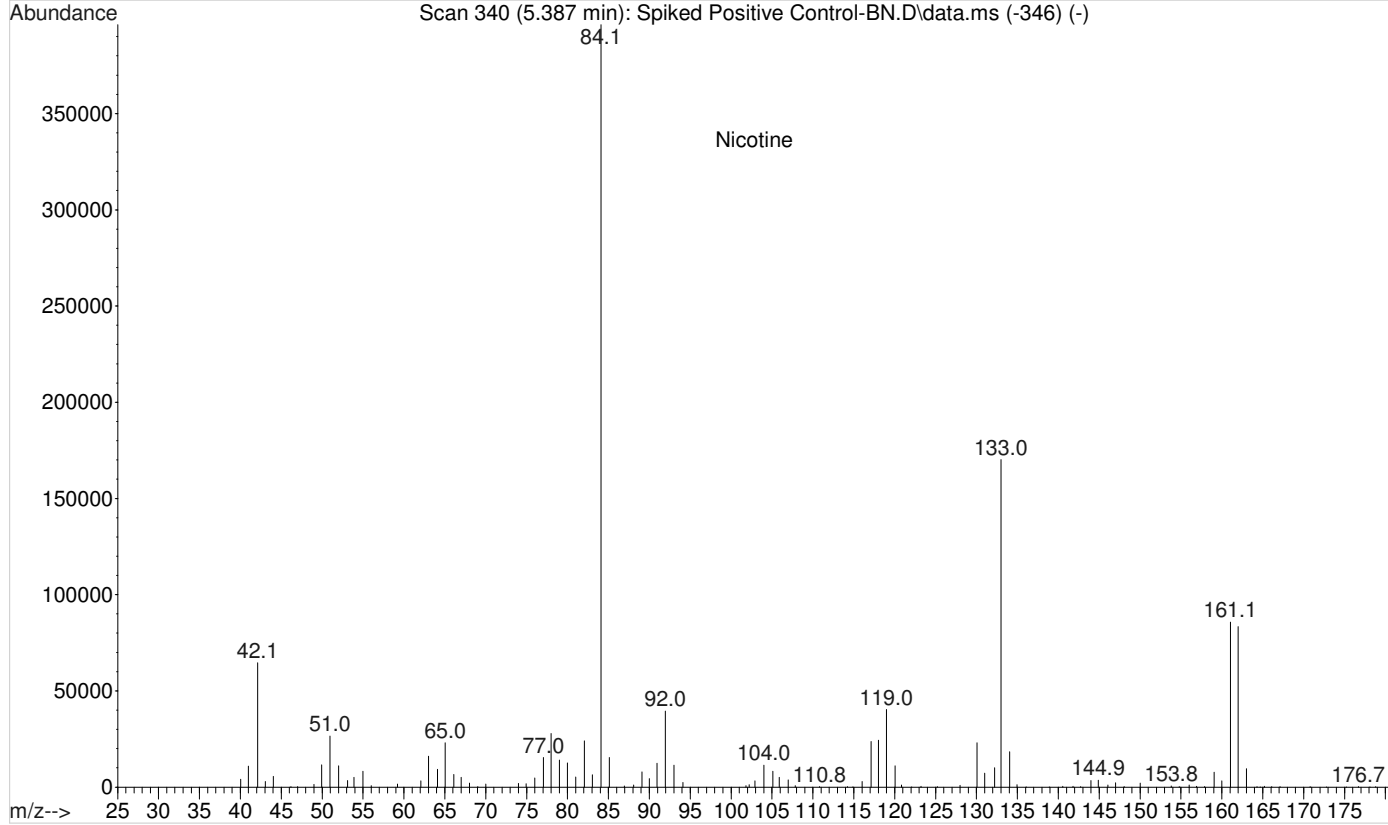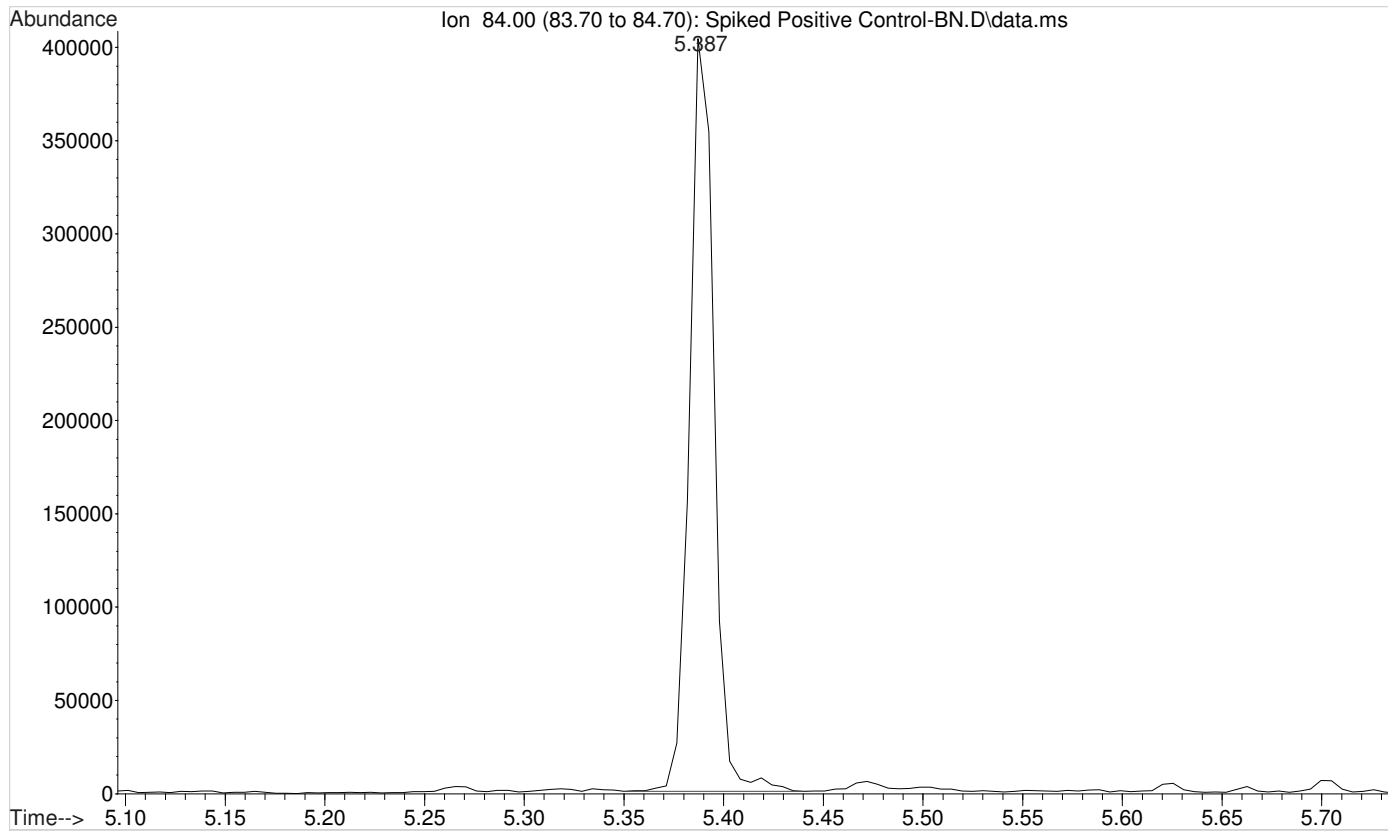



File :C:\MyFiles\cshrum\Desktop\101515 Data\Spiked Positive Contro
... l-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 15 Oct 2015 20:18 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

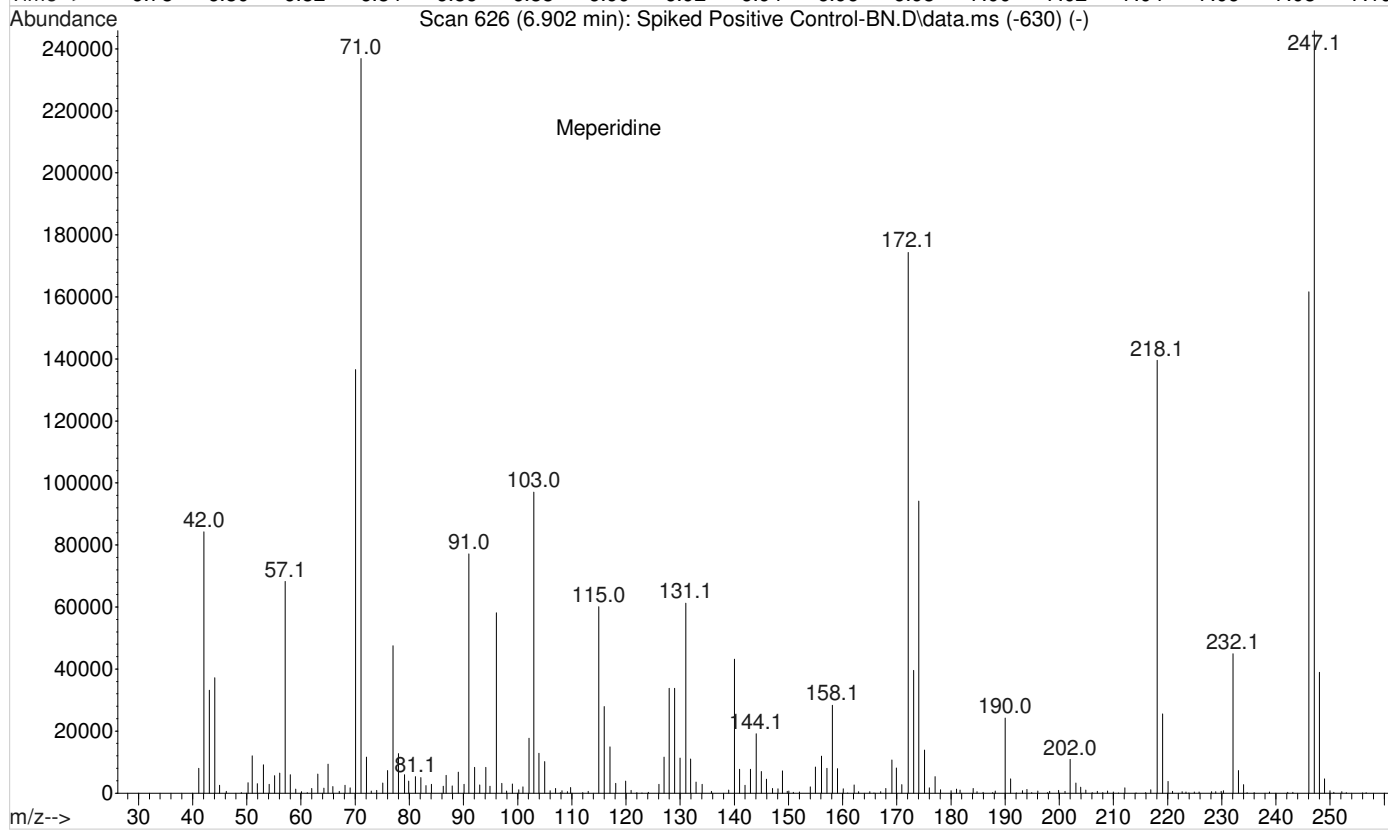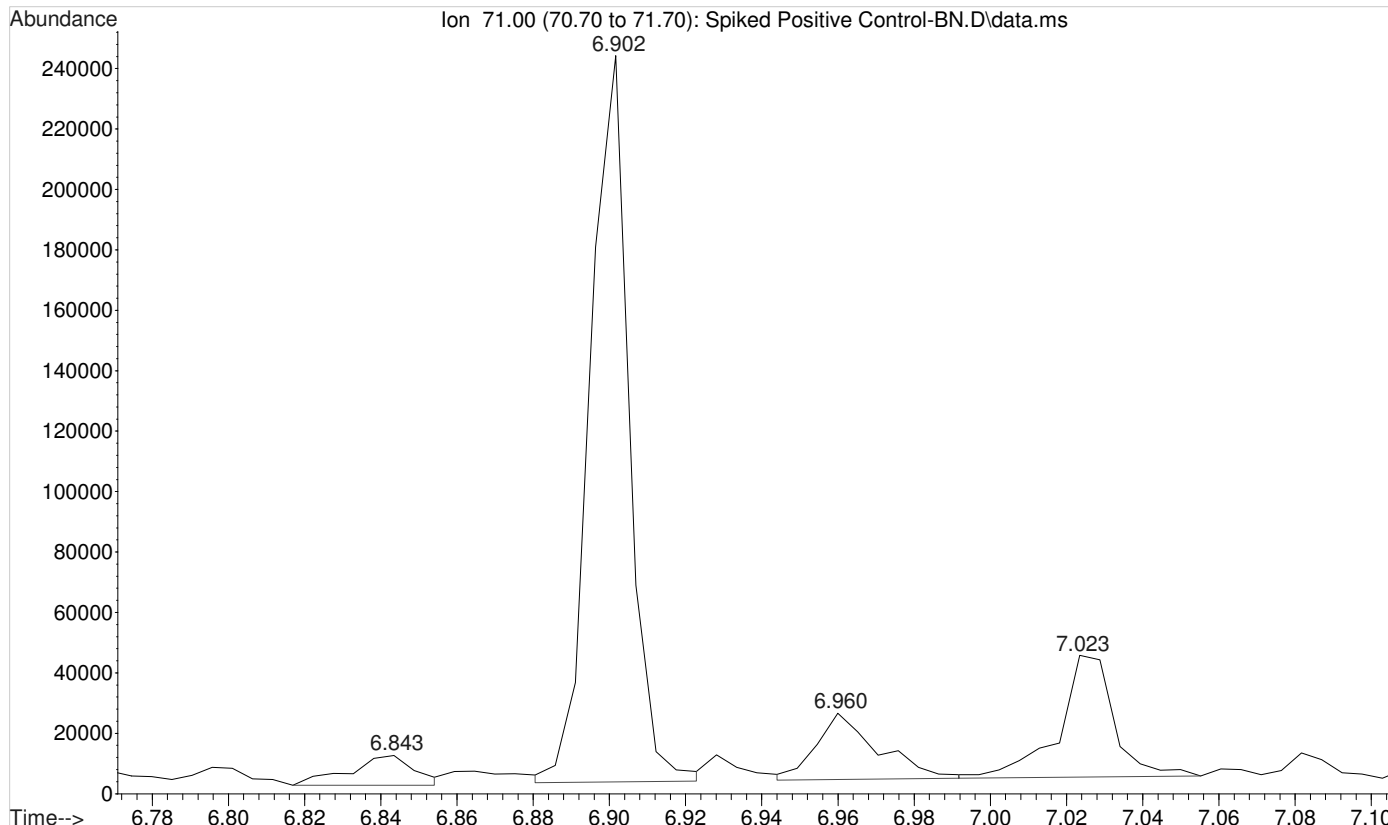


File :C:\MyFiles\cshrum\Desktop\101515 Data\Spiked Positive Contro
... l-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 15 Oct 2015 20:18 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

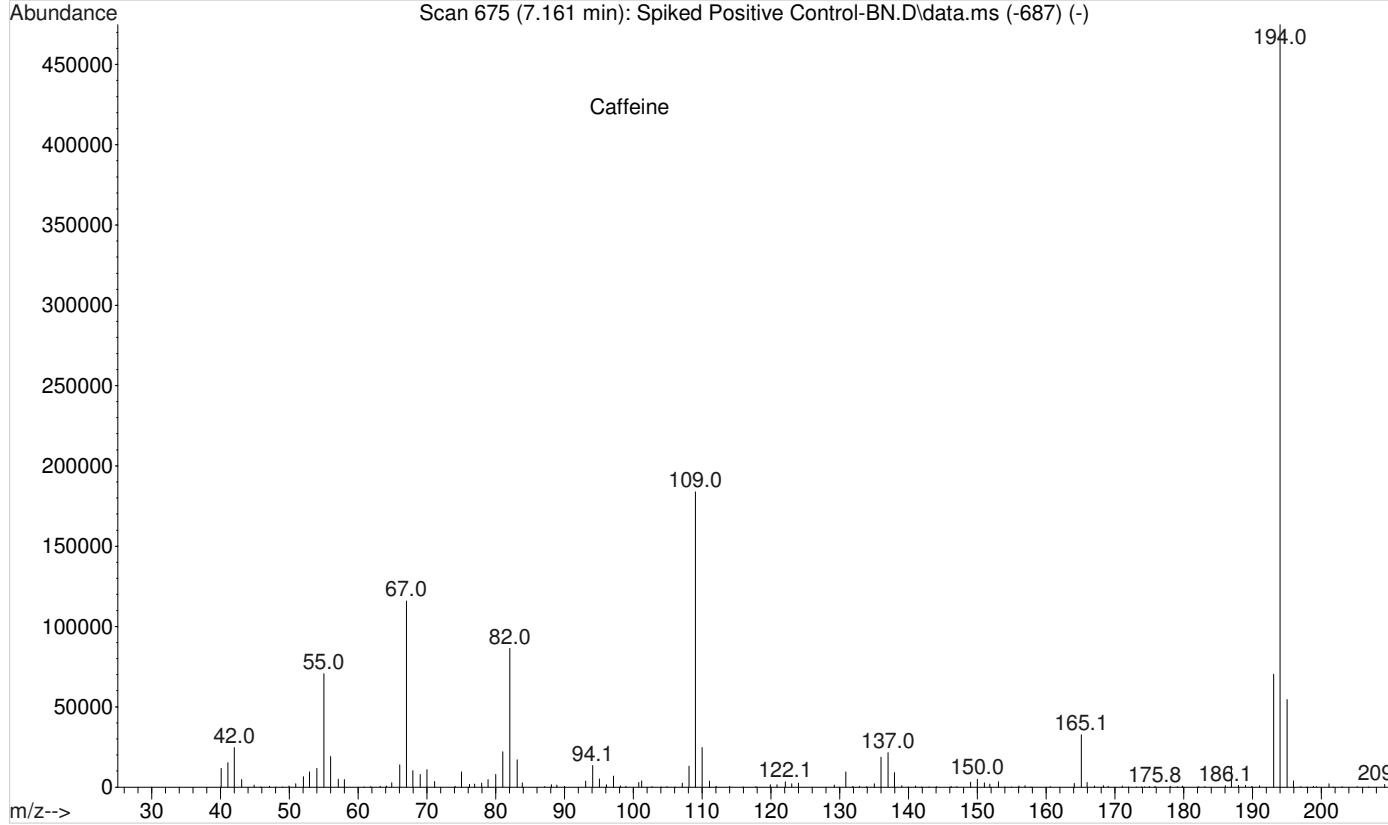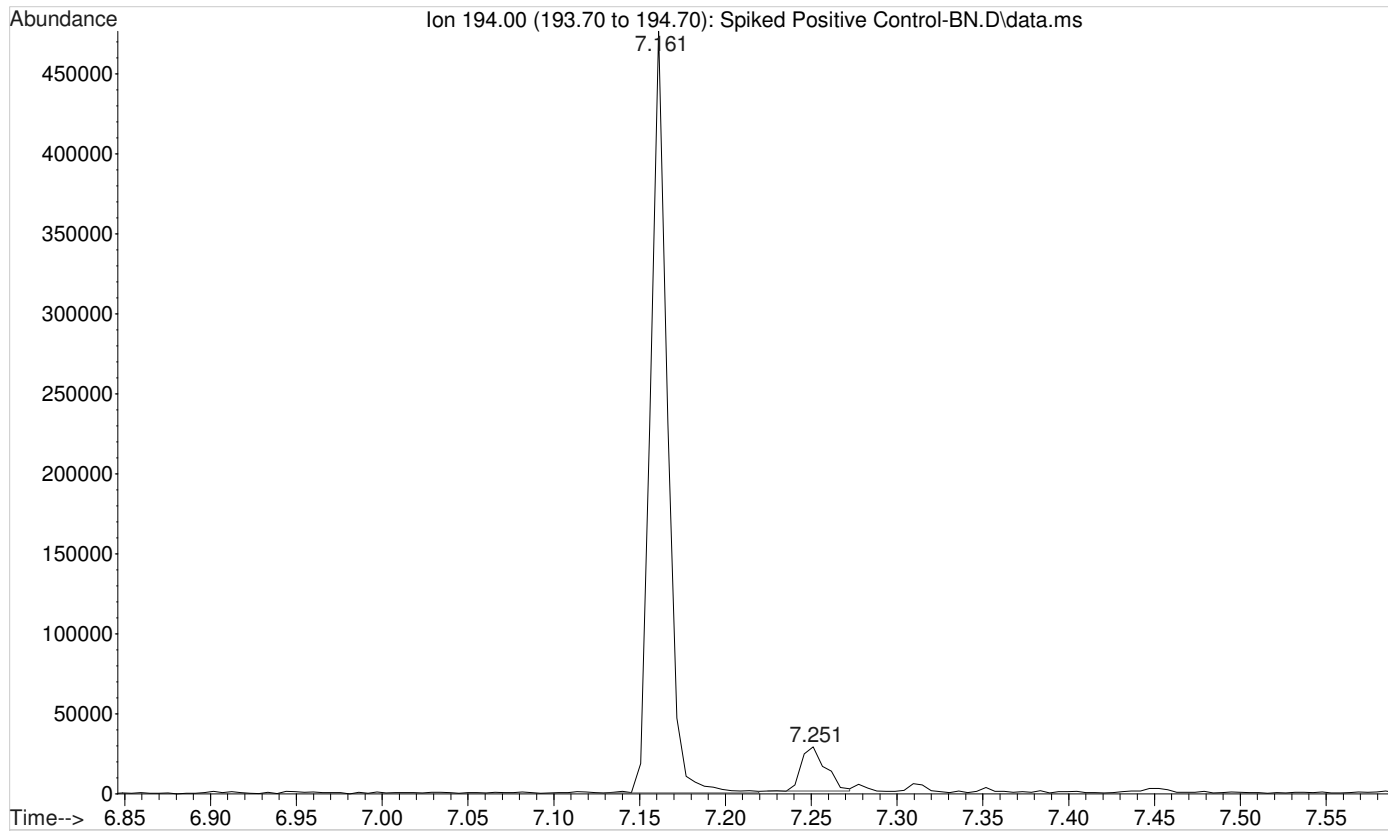

File :C:\MyFiles\cshrum\Desktop\101515 Data\Spiked Positive Contro
... l-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 15 Oct 2015 20:18 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

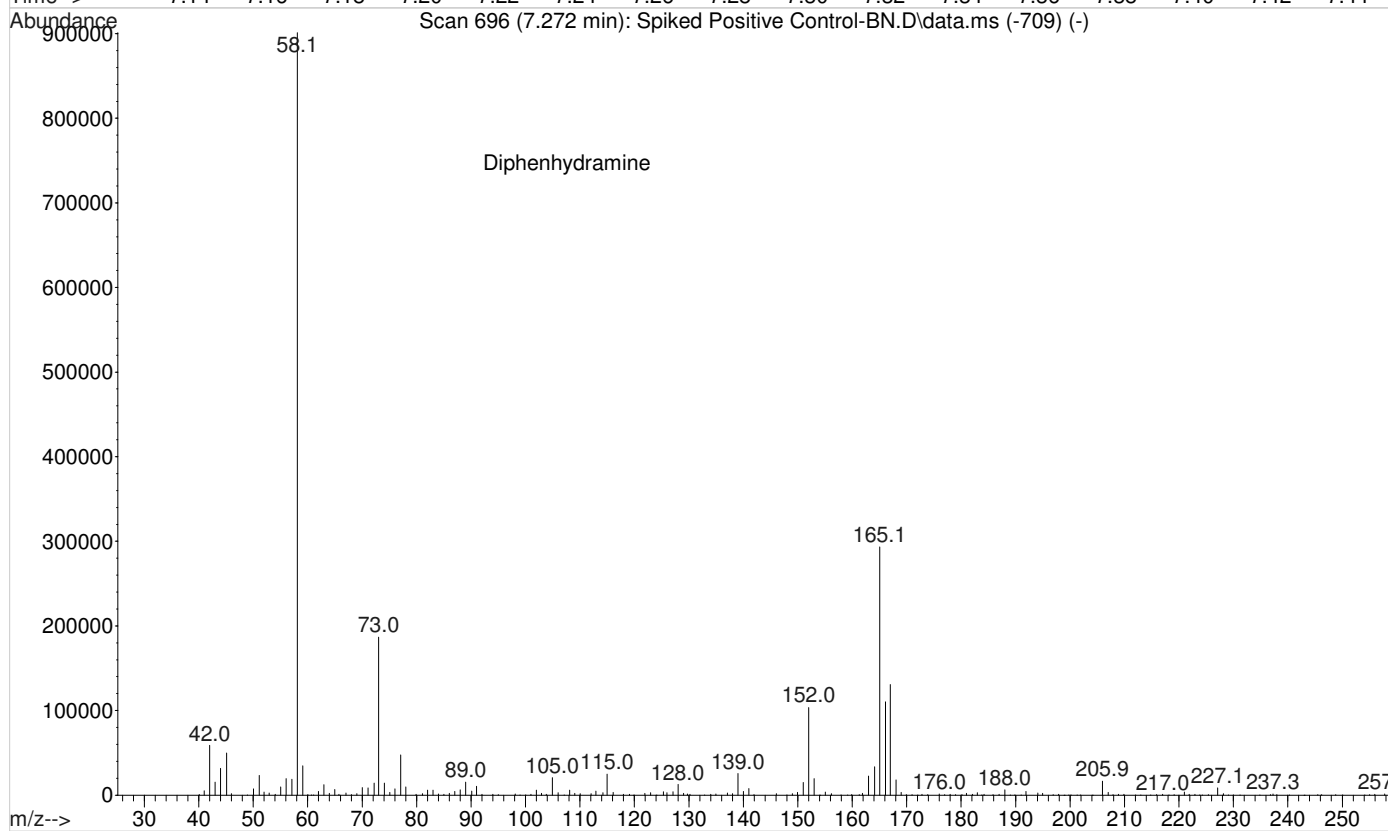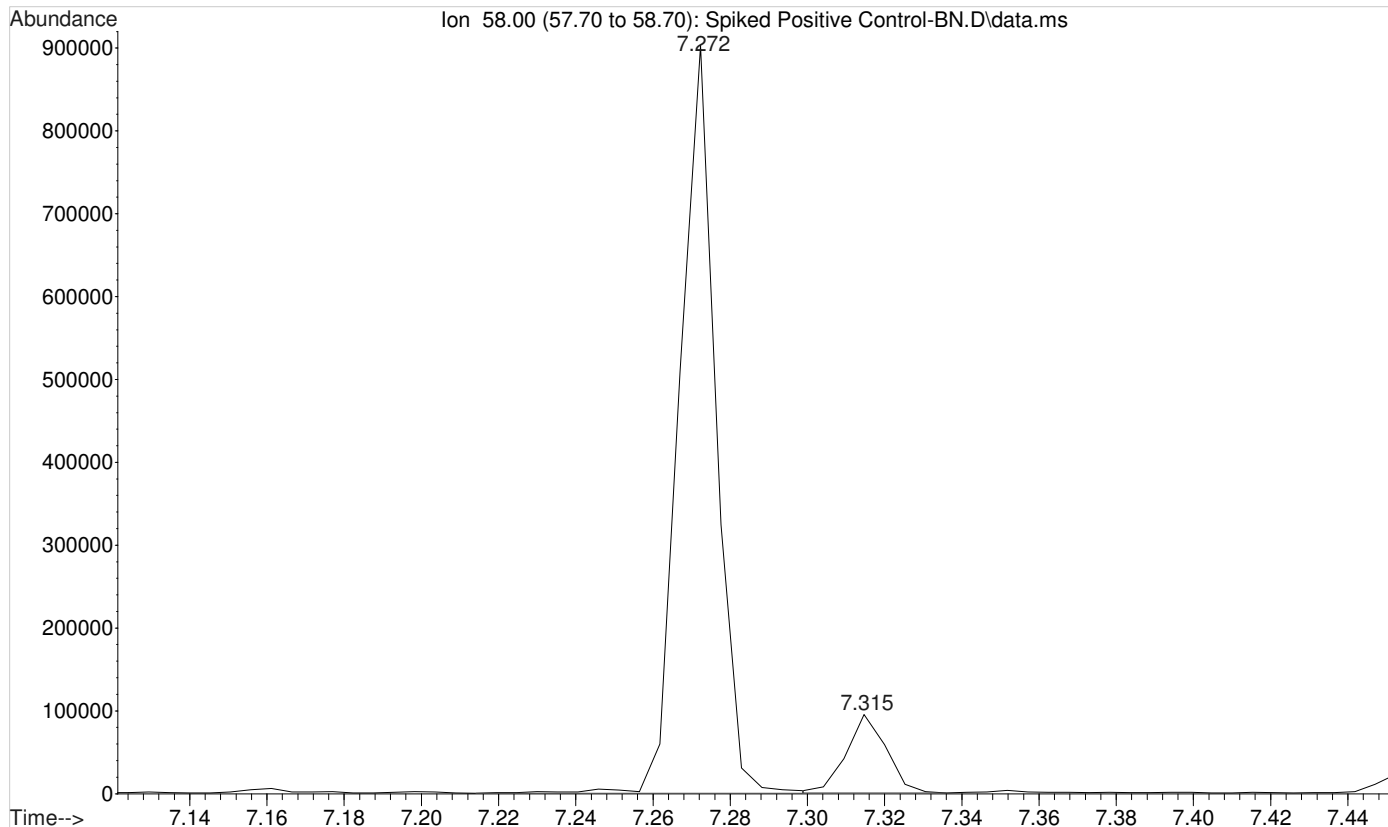

File :C:\MyFiles\cshrum\Desktop\101515 Data\POSTBLK.D
Operator : ISP\datastor
Acquired : 18 Oct 2015 00:08 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: BLK
Misc Info : Chloroform
Vial Number: 73

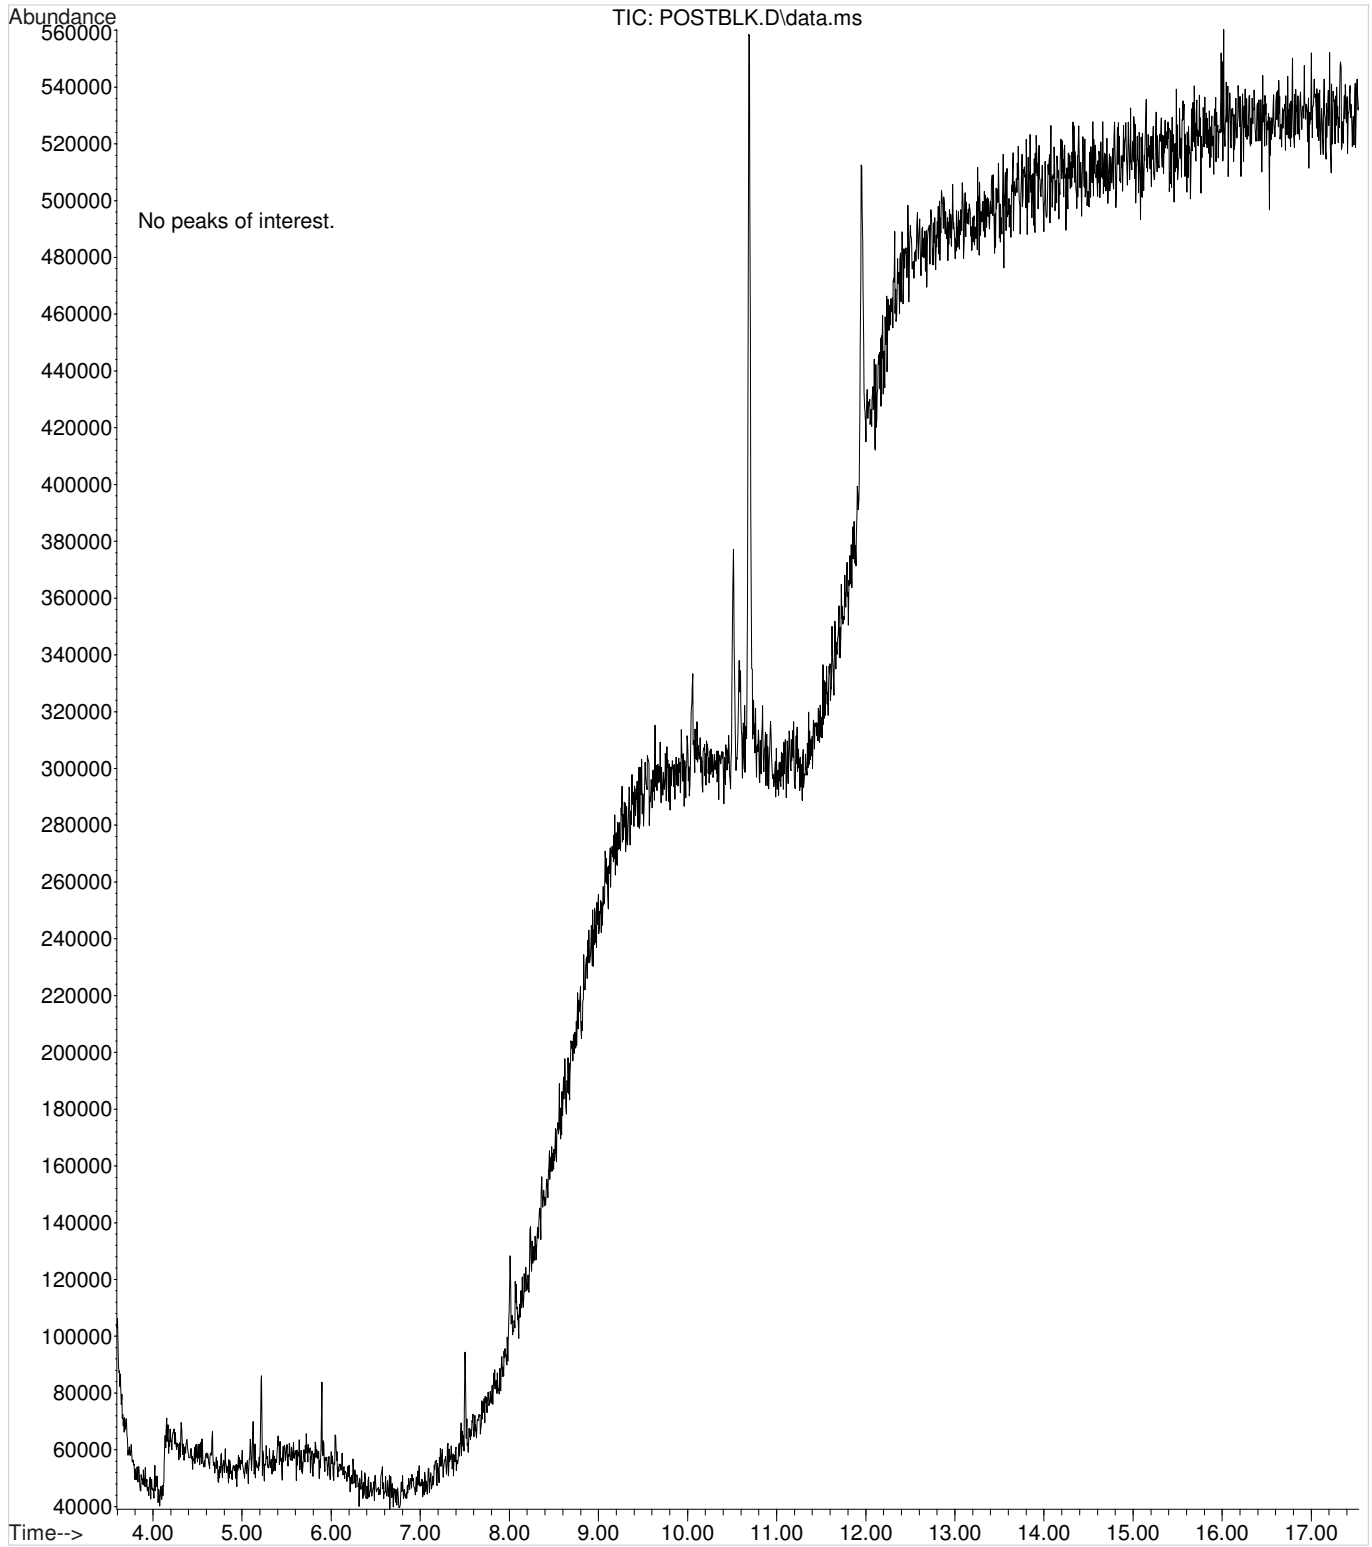

Analytical Method 3.6.1 & 3.6.7 QA Check List

Run Start Date: 10/15/15

Analyst: CS

(Long GC/MS temperature program)

Positive Control Compound List

- Methamphetamine
- Nicotine
- Meperidine
- Caffeine
- Diphenhydramine
- Lidocaine
- PCP
- Methadone
- Amitriptyline
- Codeine
- Trazodone



Internal Standards

- Benzphetamine
- Papaverine



Optional back extraction **not** performed.
Reconstituted in MeOH.

Phentermine was also added. ☺


File :C:\MyFiles\cshrum\Desktop\101515 Data\Prerun Solvent Blankr.D
Operator : ISP\datastor
Acquired : 15 Oct 2015 21:04 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Pre-run Solvent Blank
Misc Info : Chloroform
Vial Number: 100

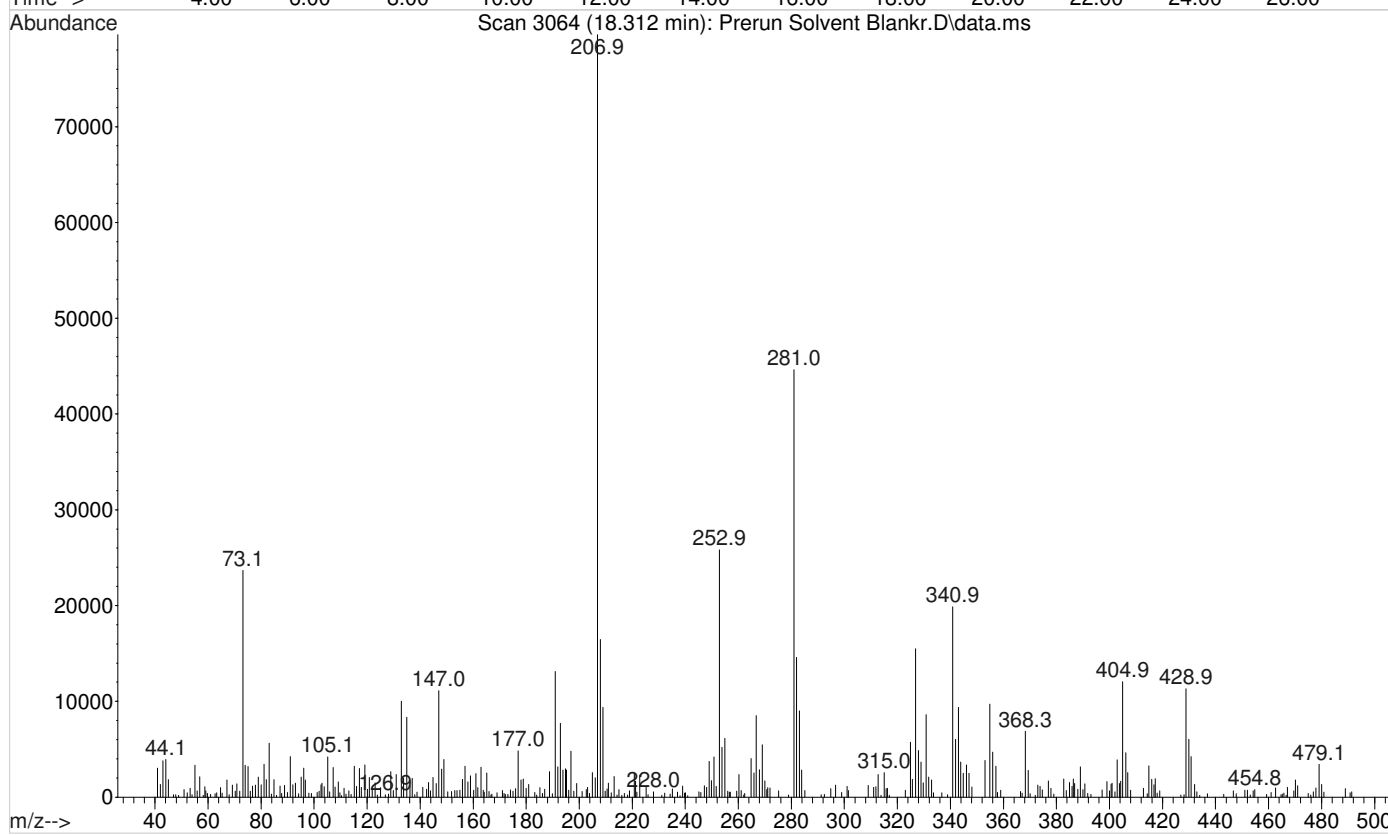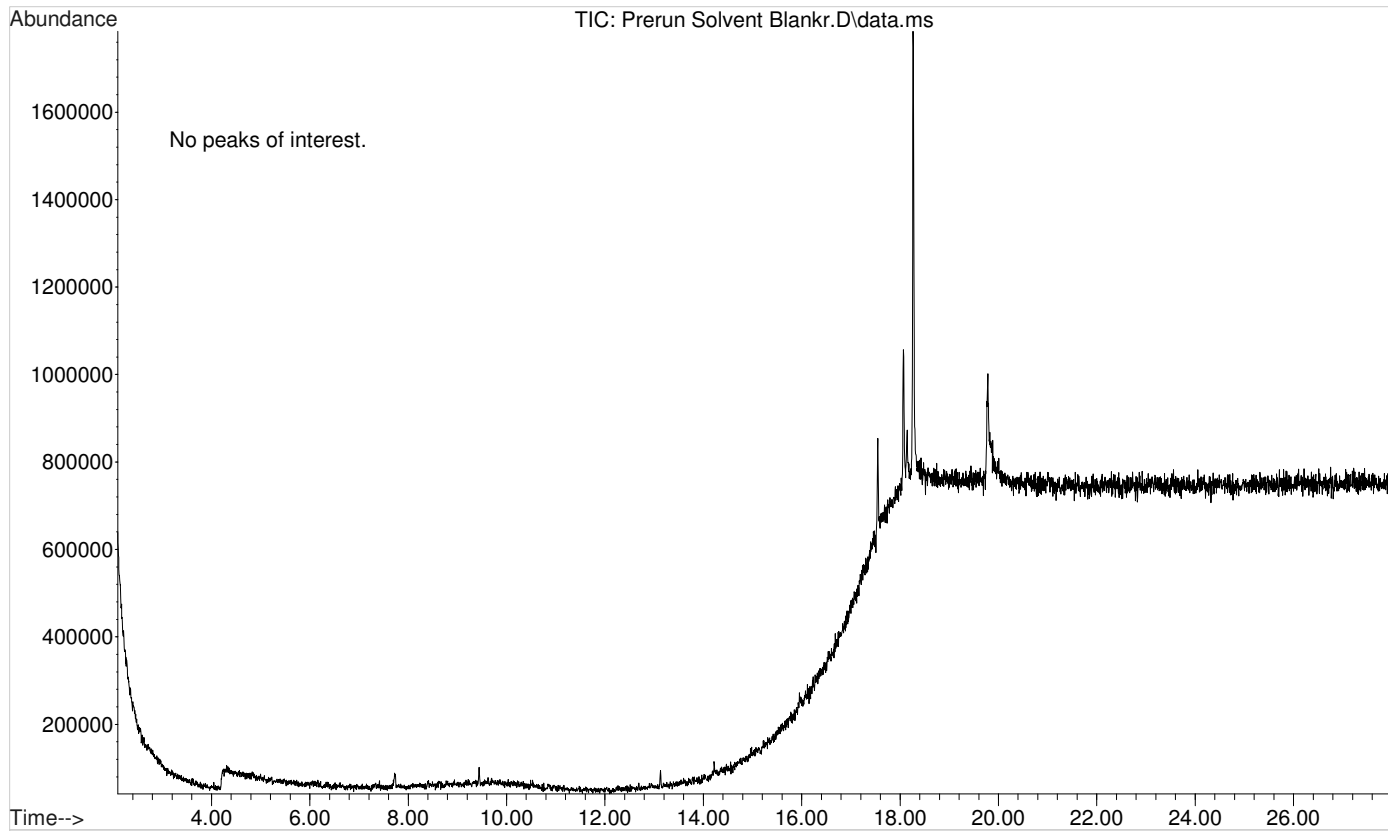



File :C:\MyFiles\cshrum\Desktop\101515 Data\prbLK2r.D
Operator : ISP\datastor
Acquired : 15 Oct 2015 22:50 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Solvent Blank
Misc Info : Chloroform
Vial Number: 99

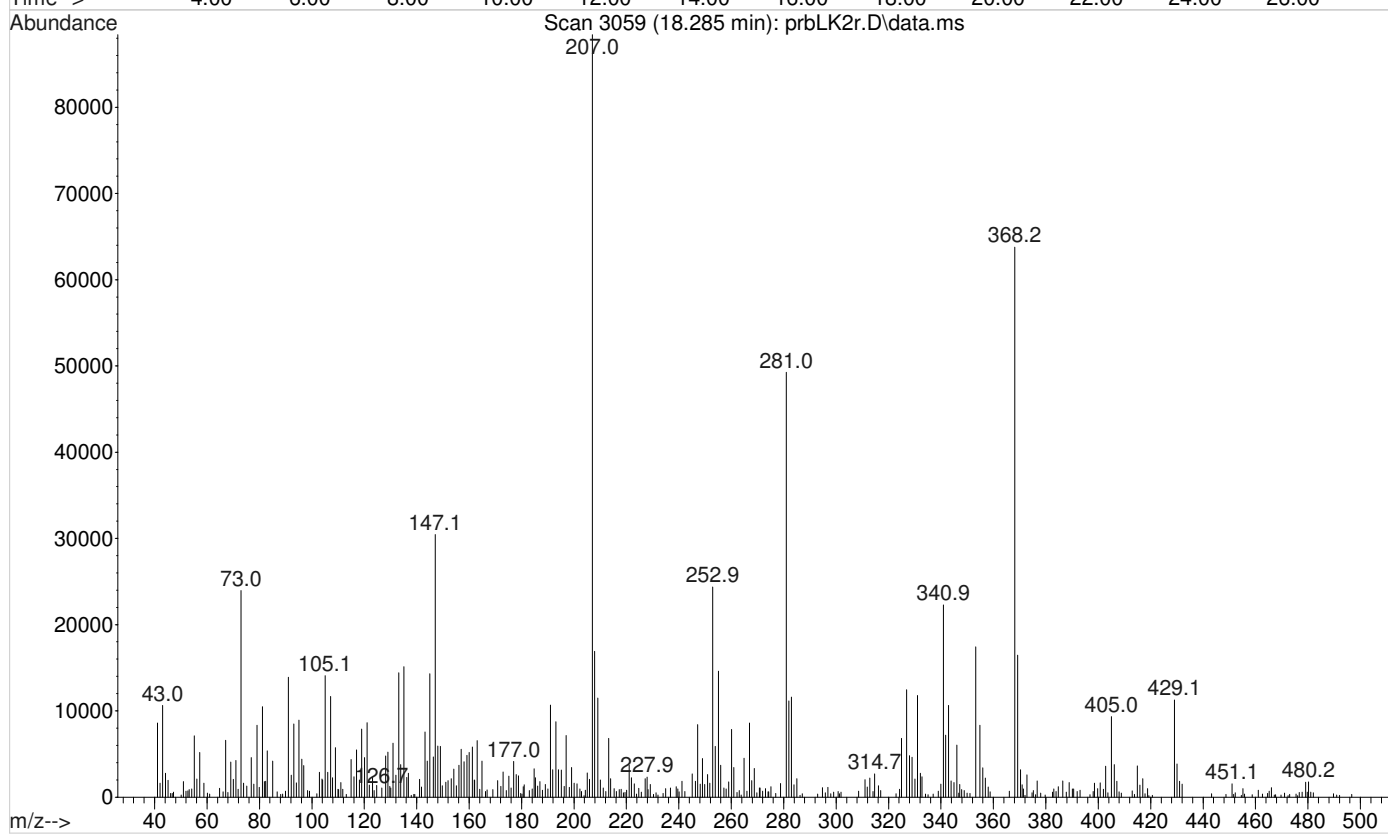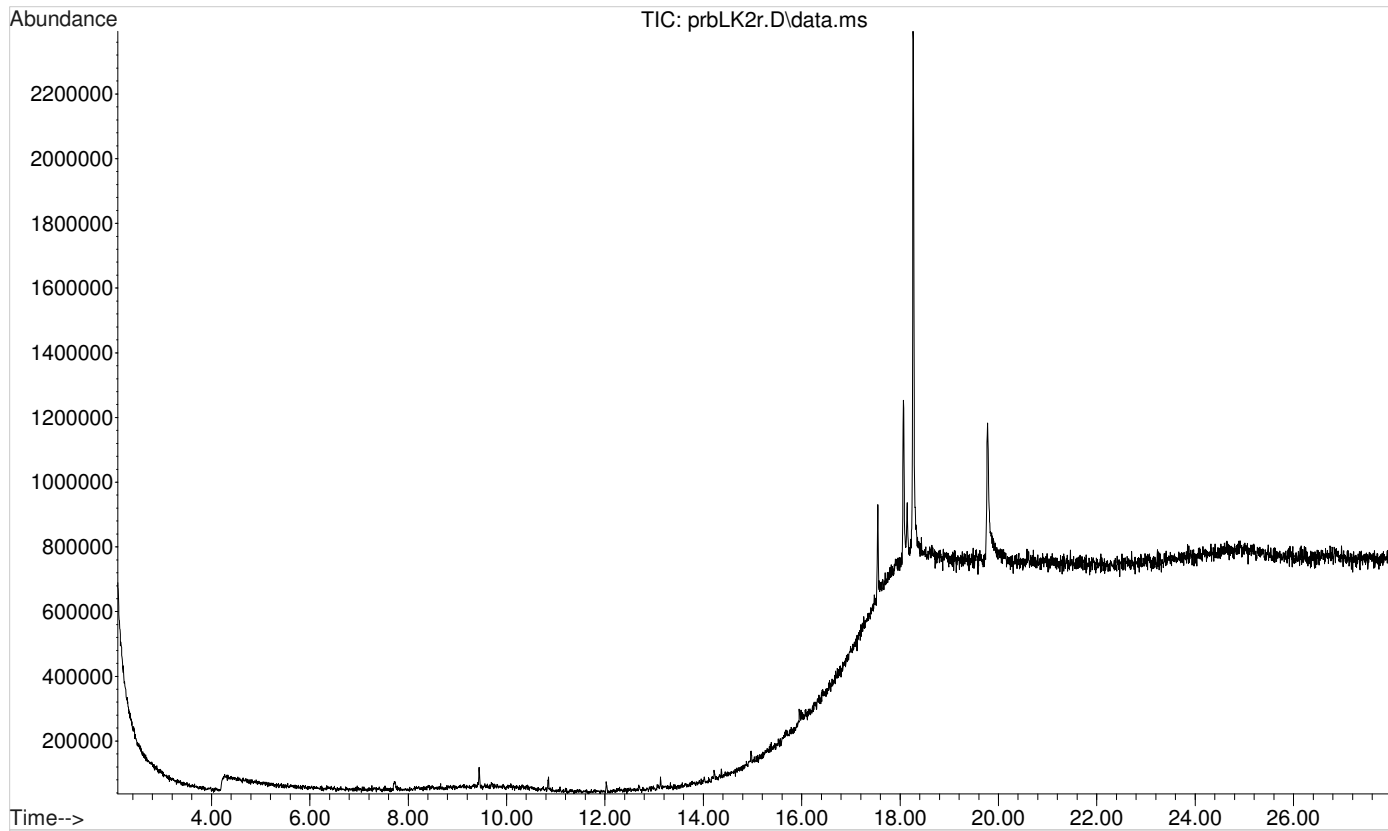



File :C:\MyFiles\cshrum\Desktop\101515 Data\Negative Control-BNr.D
Operator : ISP\datastor
Acquired : 15 Oct 2015 21:40 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1
Vial Number: 1

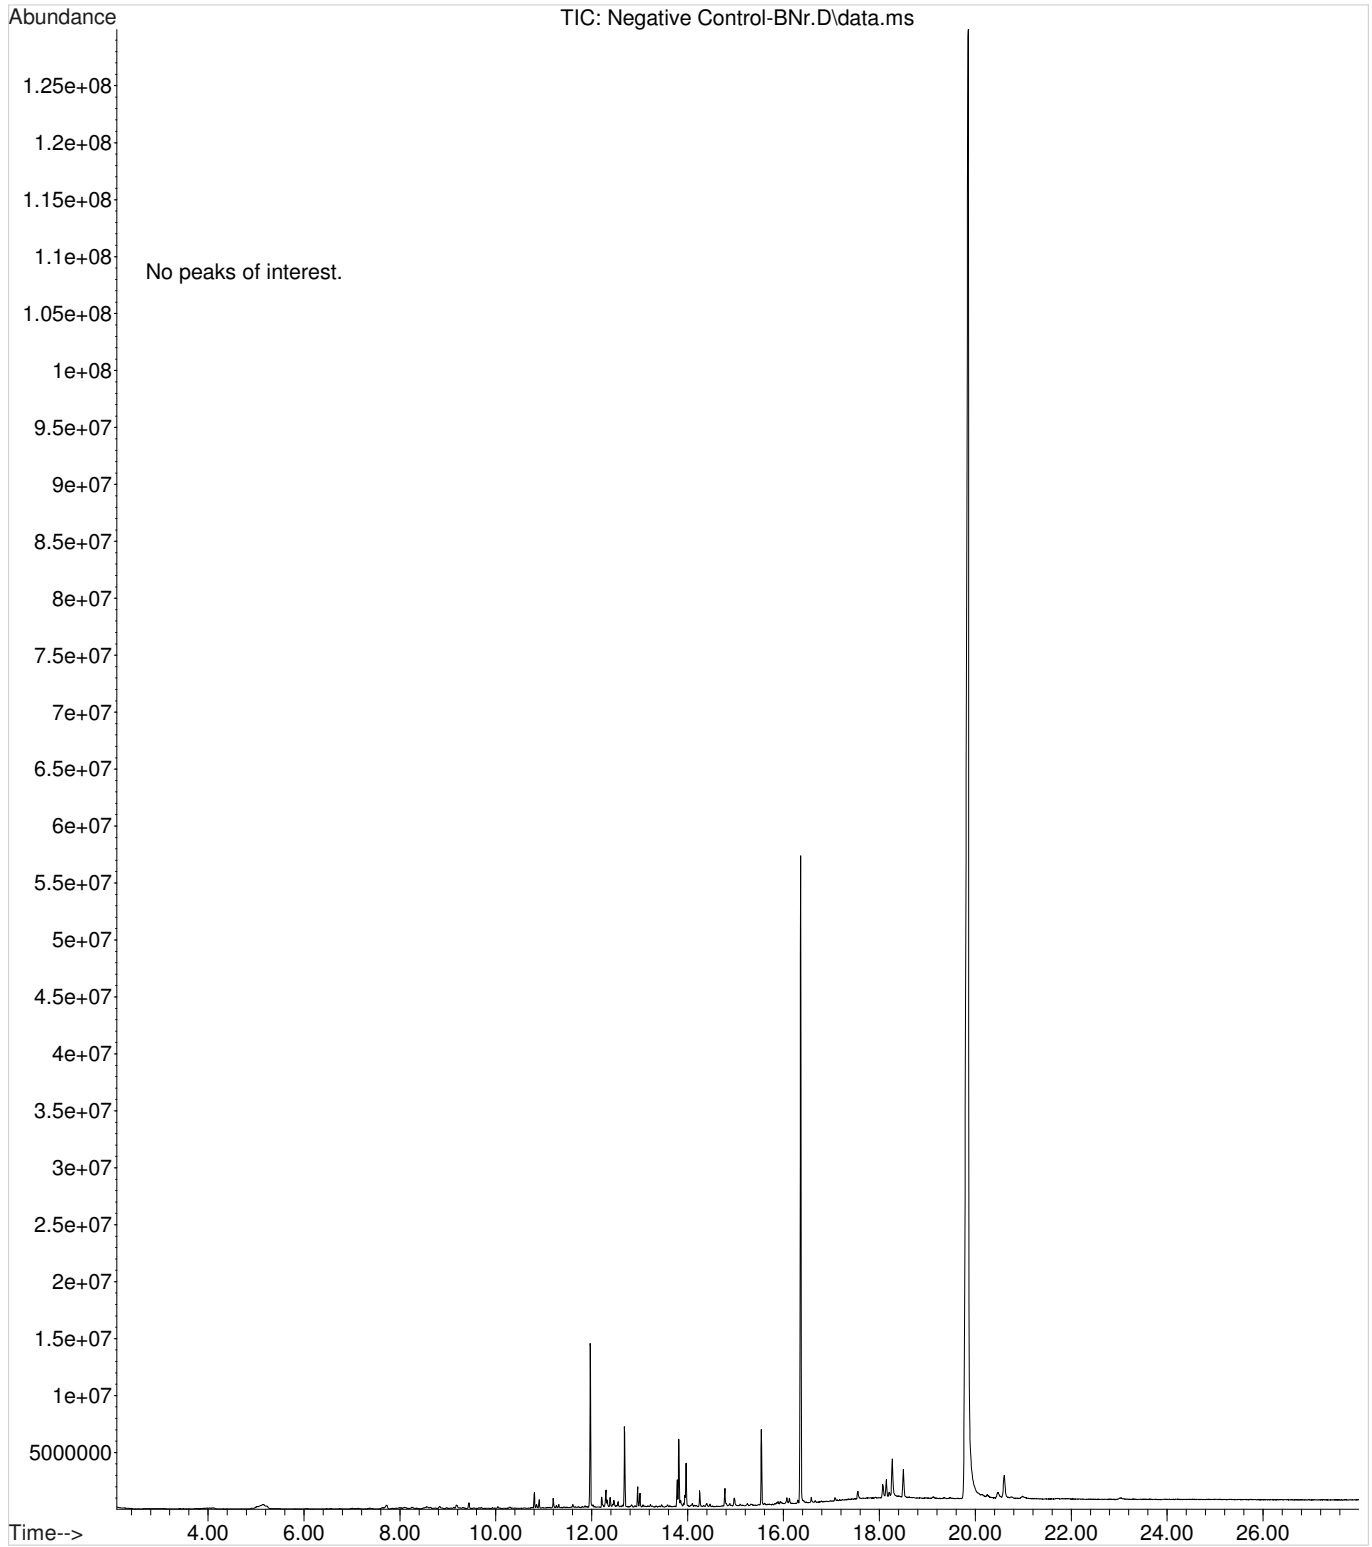


File :C:\MyFiles\cshrum\Desktop\101515 Data\Negative Control-BNr.D
Operator : ISP\datastor
Acquired : 15 Oct 2015 21:40 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1
Vial Number: 1

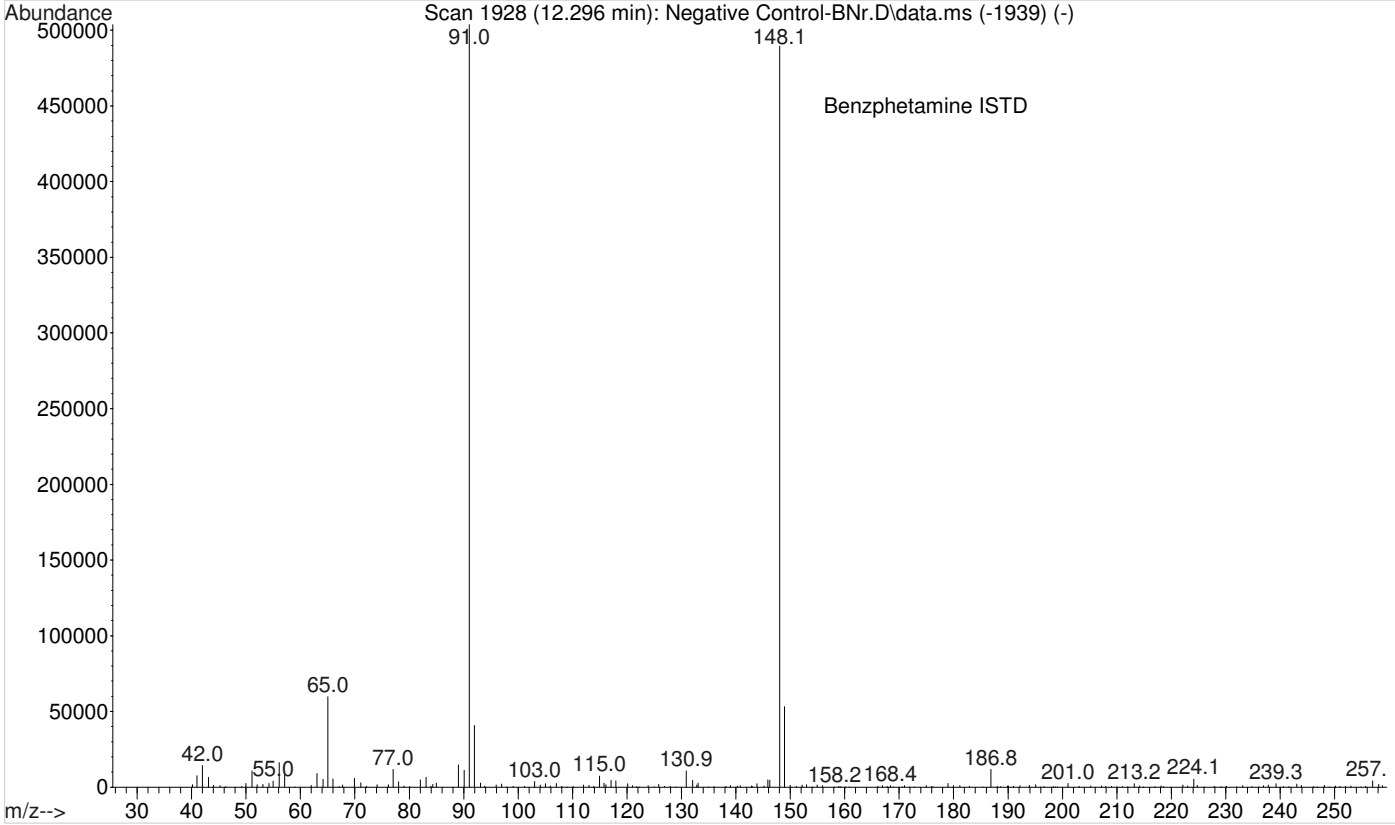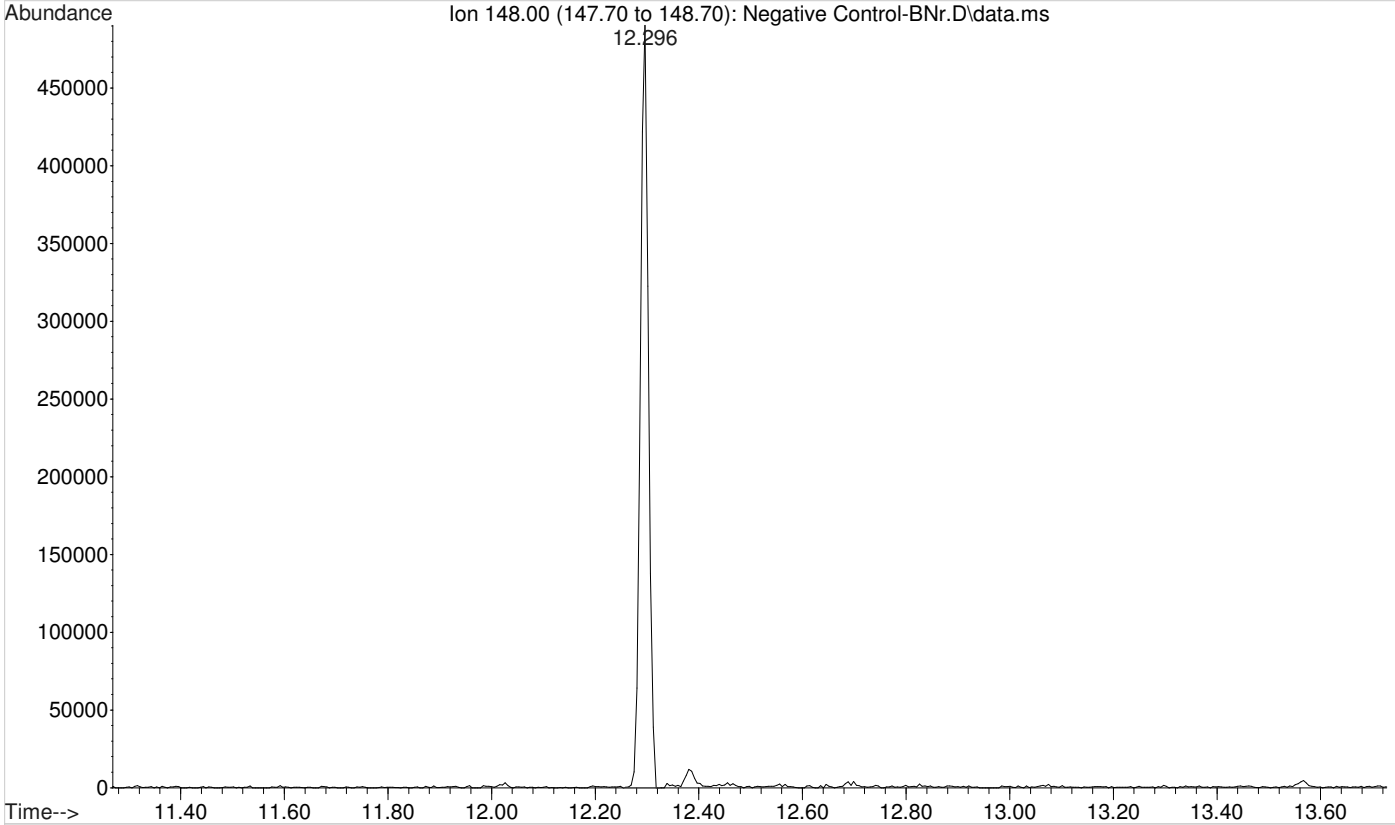



File :C:\MyFiles\cshrum\Desktop\101515 Data\Negative Control-BNr.D
Operator : ISP\datastor
Acquired : 15 Oct 2015 21:40 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1
Vial Number: 1

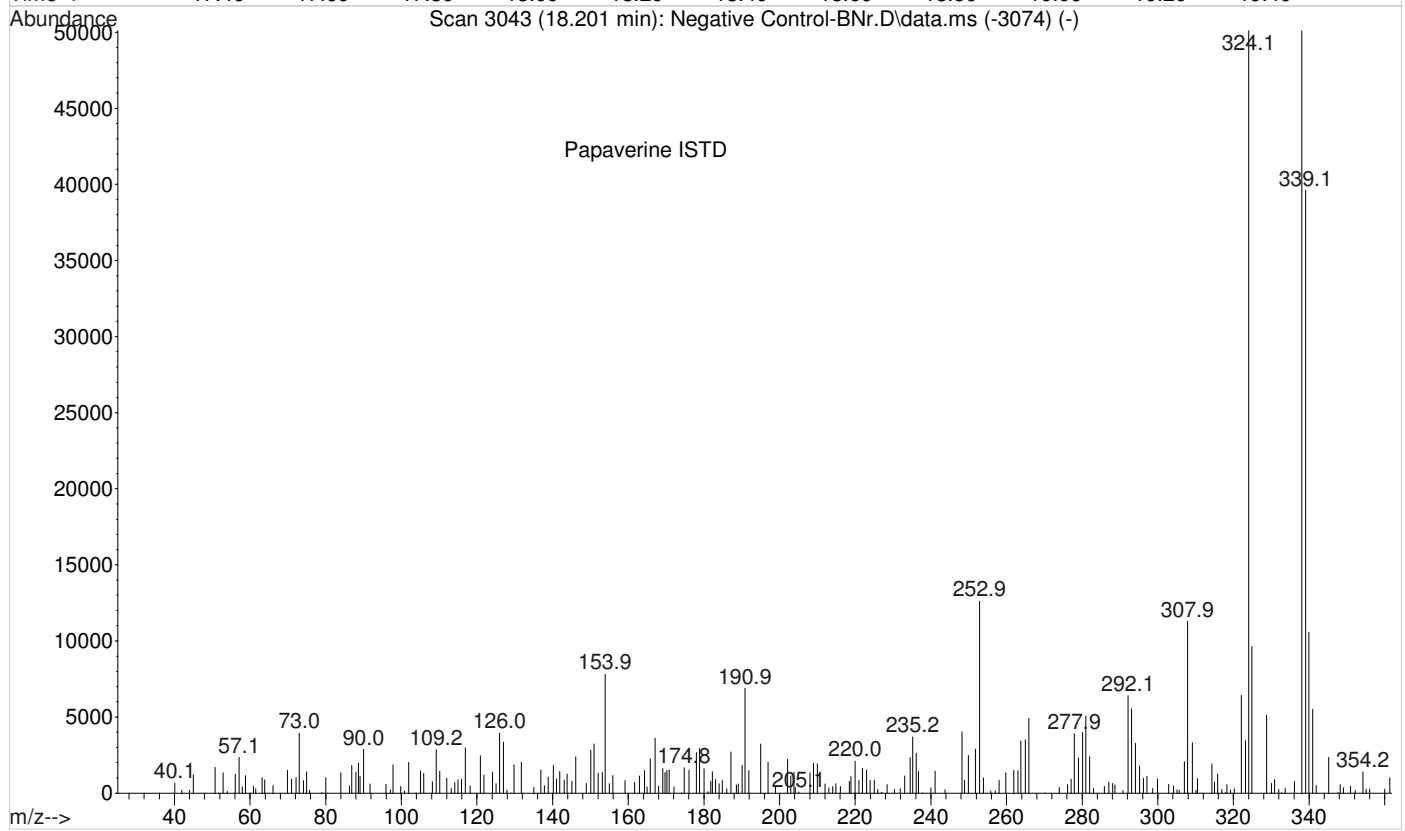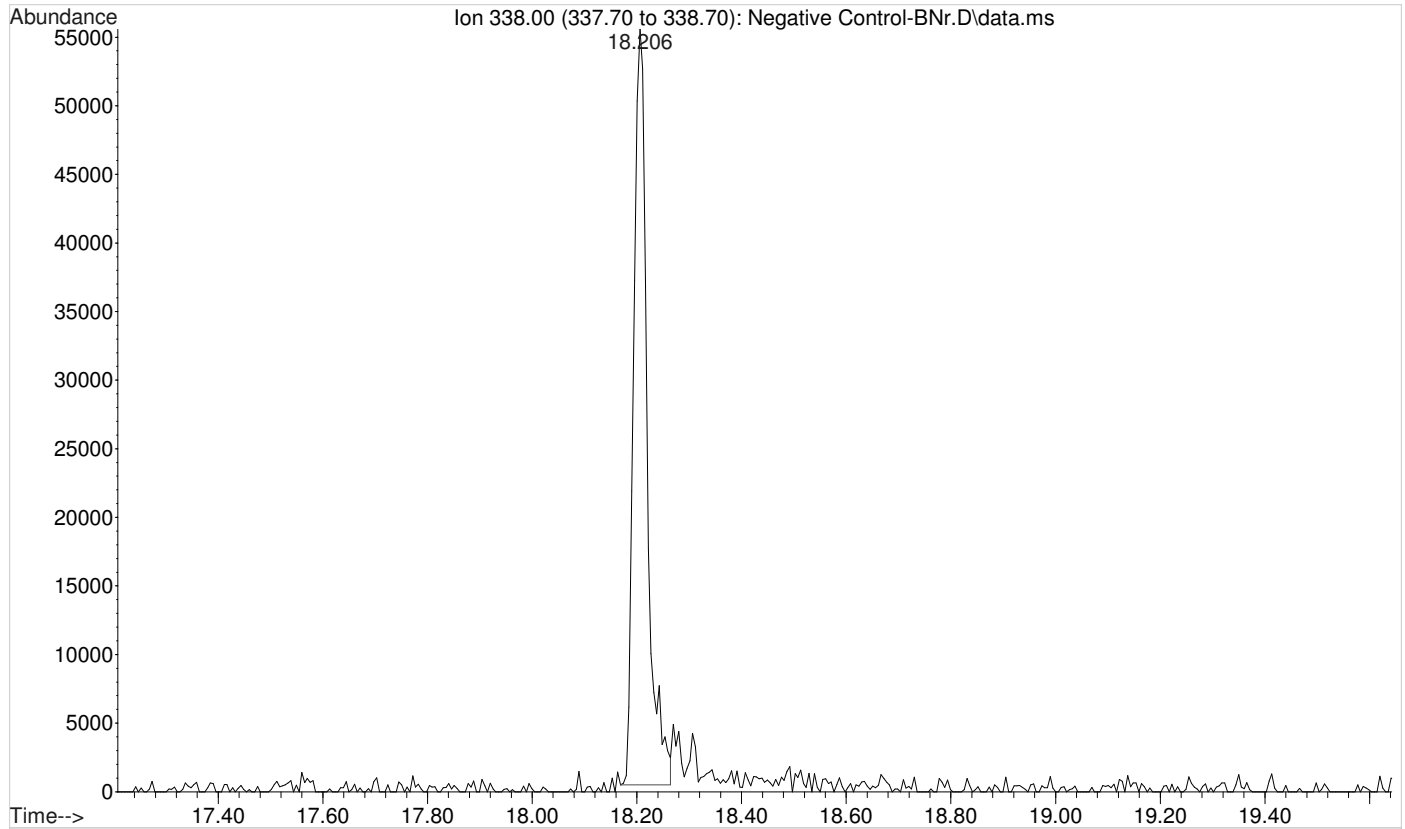



File :C:\MyFiles\cshrum\Desktop\101515 Data\Spiked Positive Contro
... l-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 15 Oct 2015 22:15 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

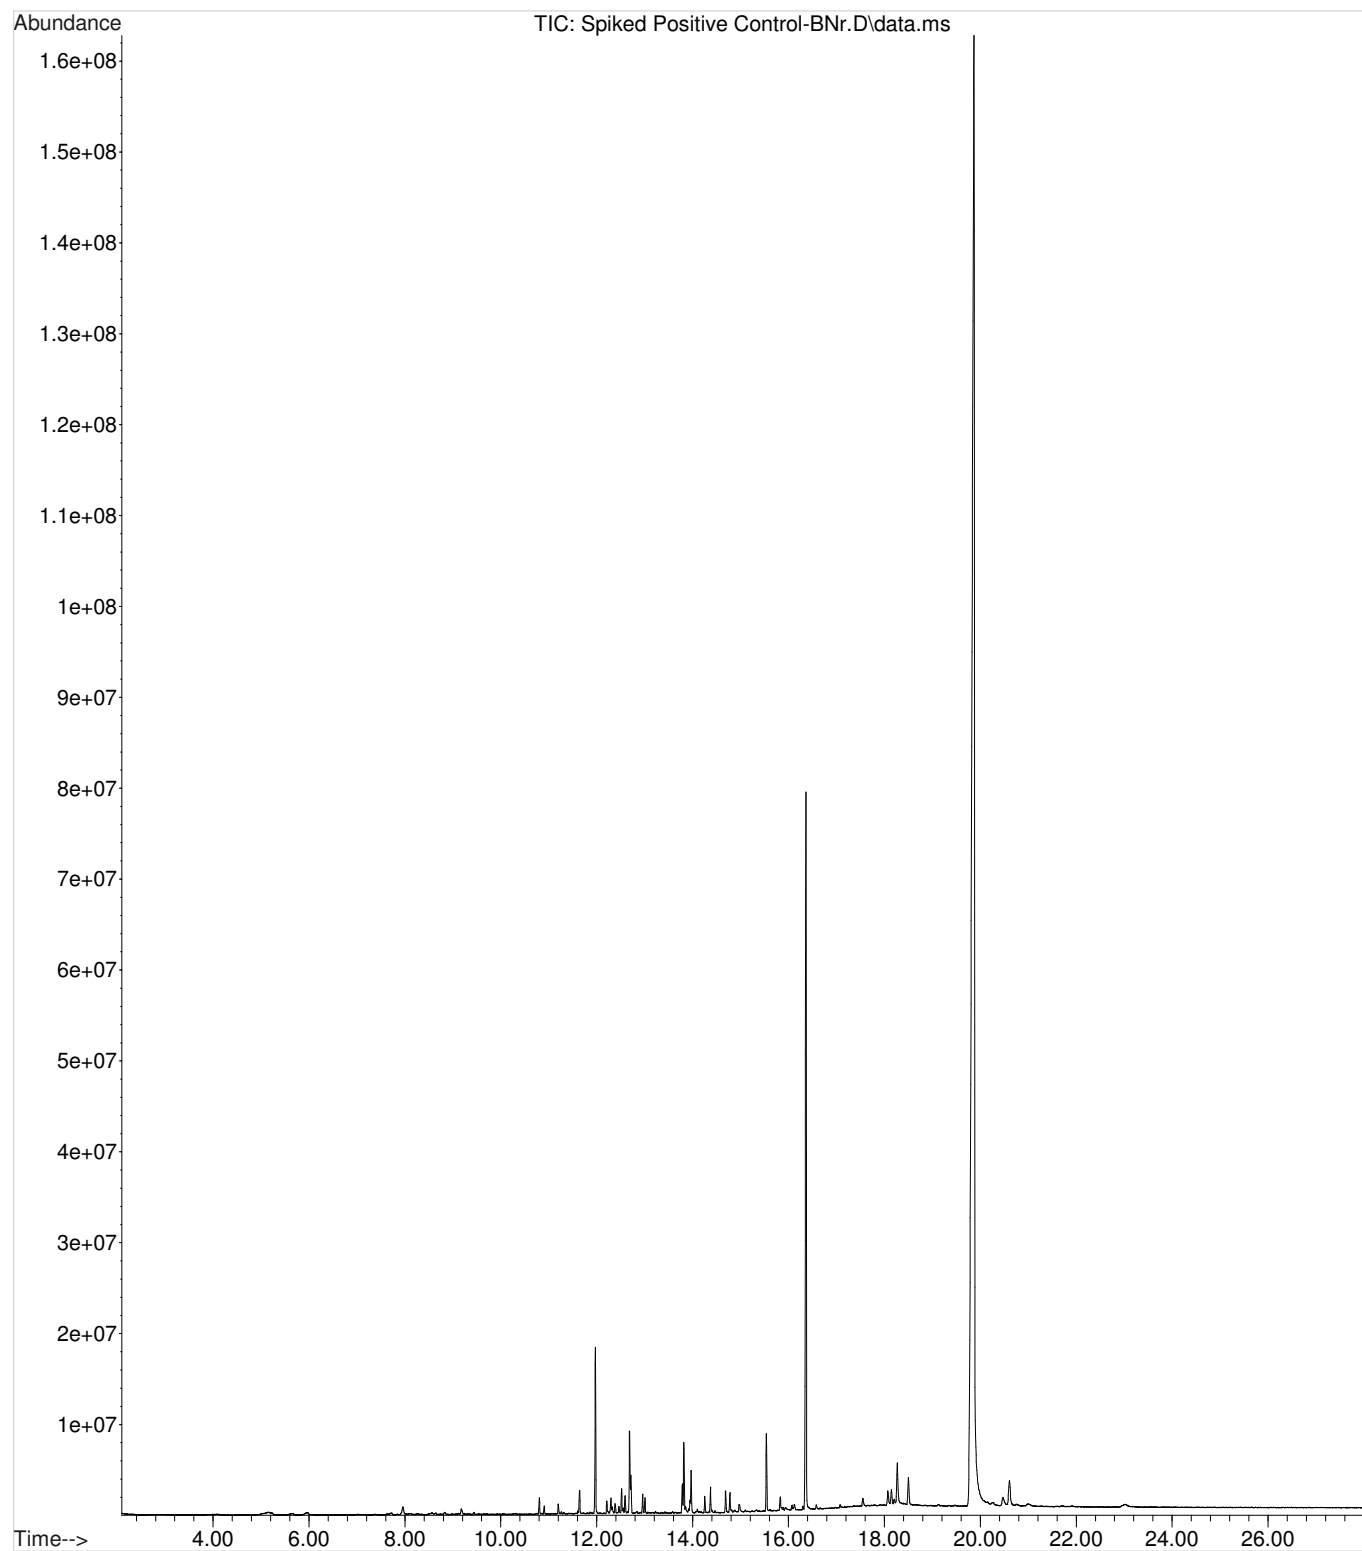



File :C:\MyFiles\cshrum\Desktop\101515 Data\Spiked Positive Control
... l-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 15 Oct 2015 22:15 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

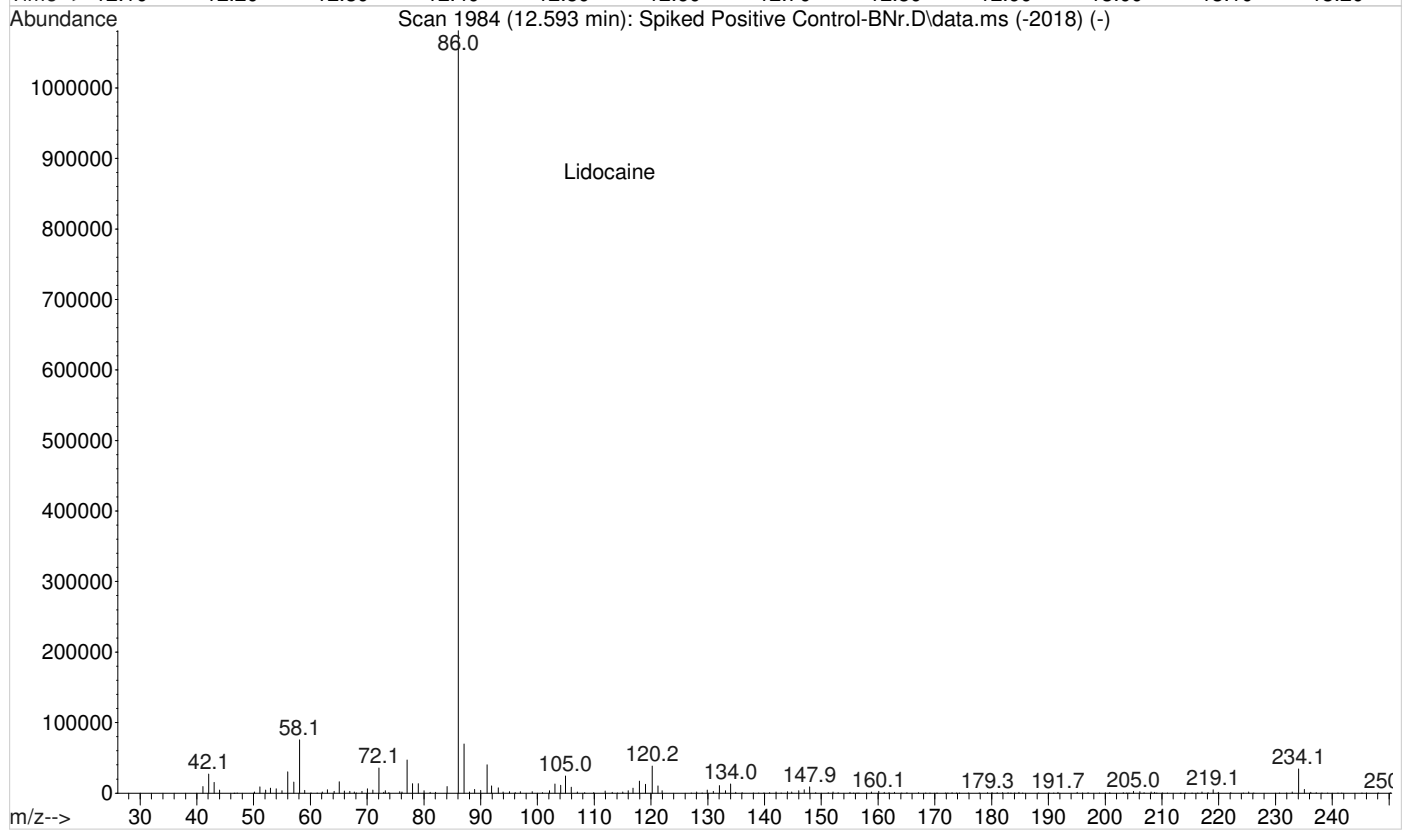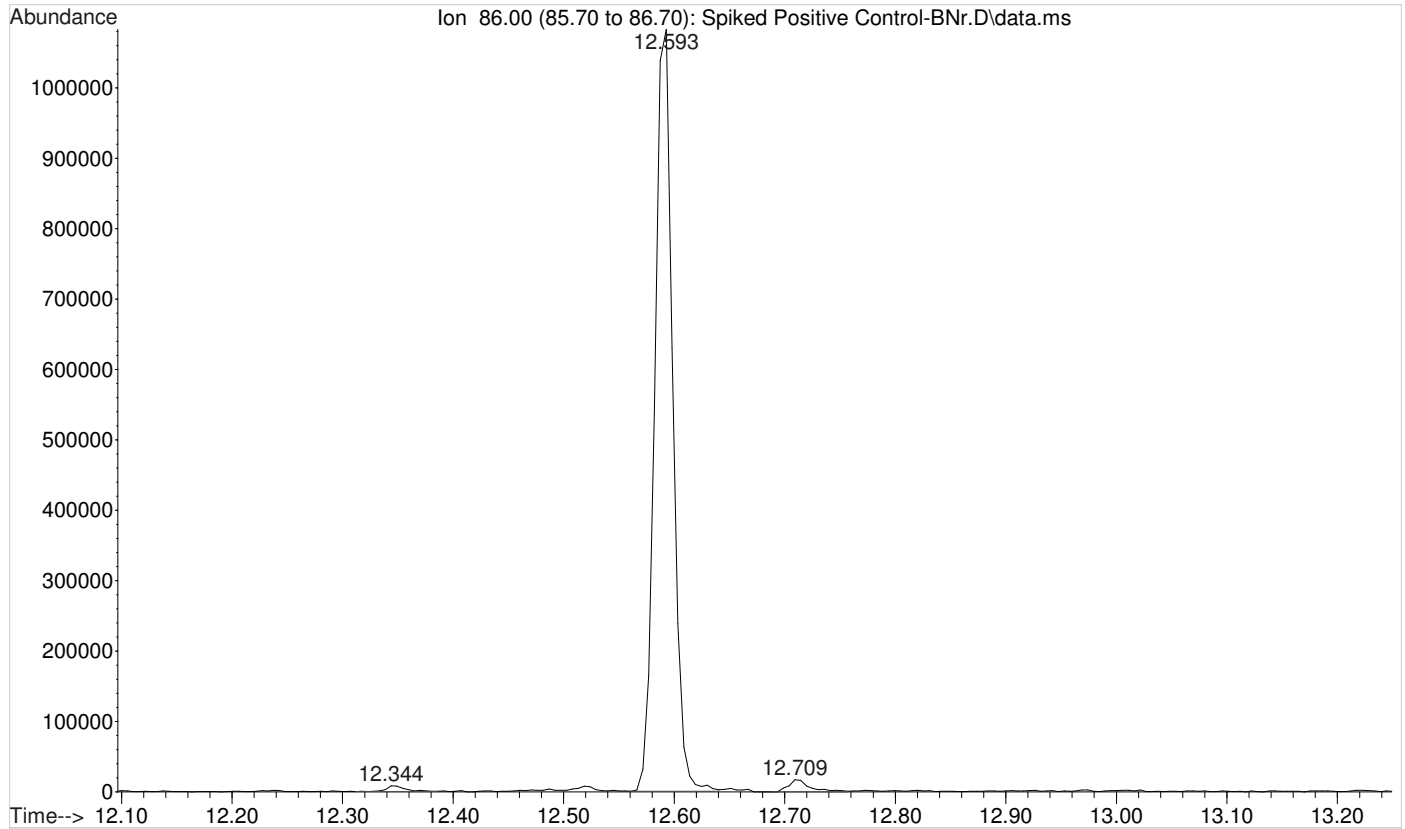



File :C:\MyFiles\cshrum\Desktop\101515 Data\Spiked Positive Contro
... l-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 15 Oct 2015 22:15 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

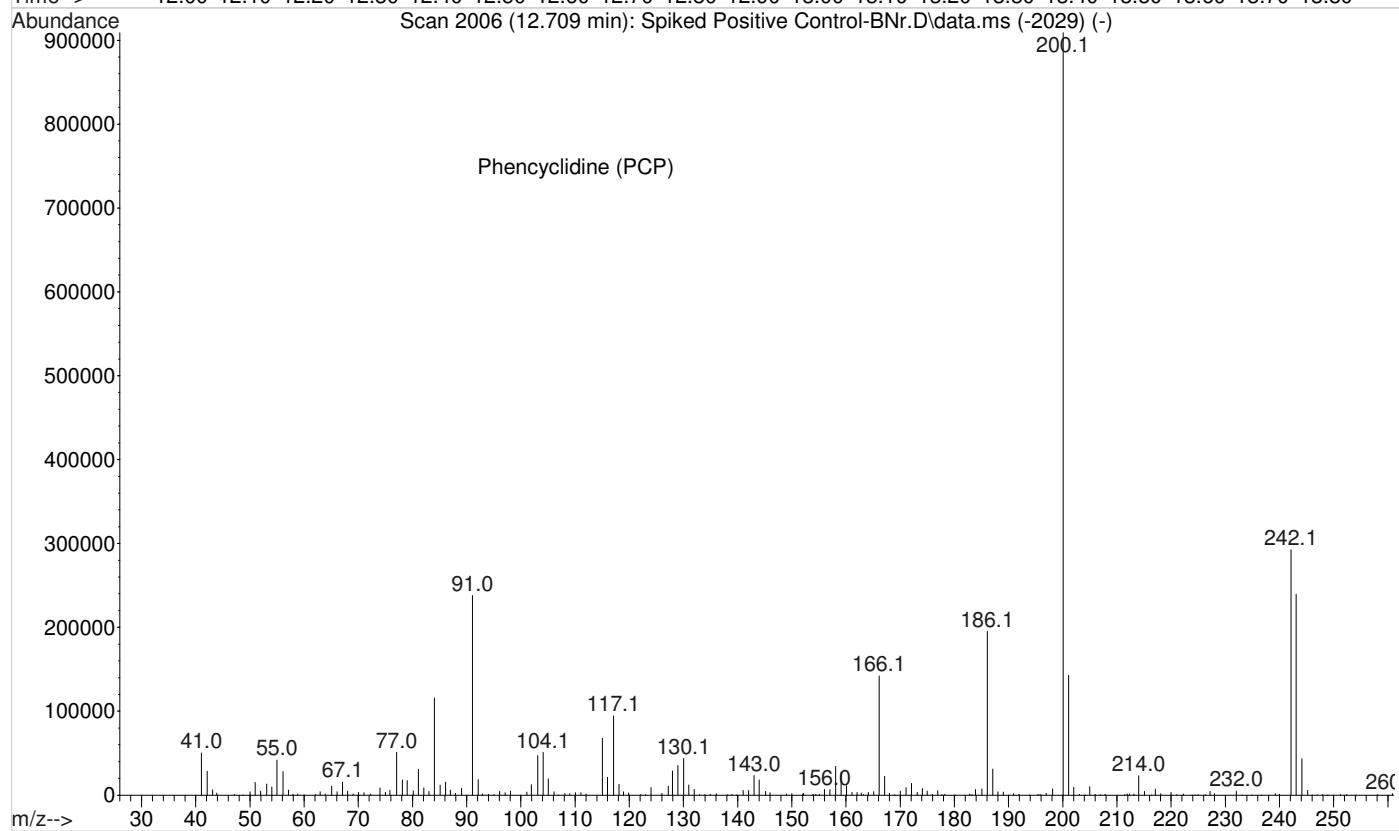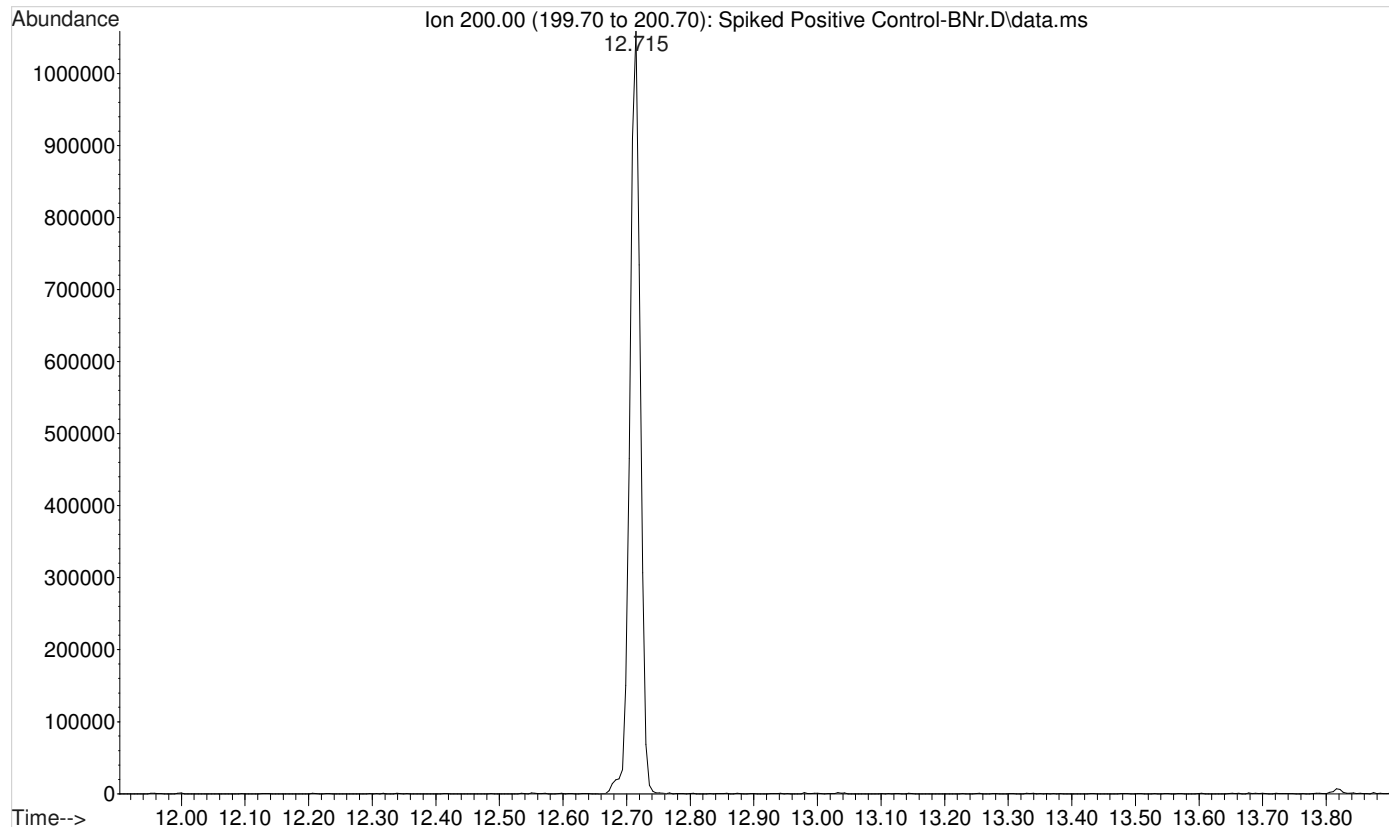



File :C:\MyFiles\cshrum\Desktop\101515 Data\Spiked Positive Control
... l-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 15 Oct 2015 22:15 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

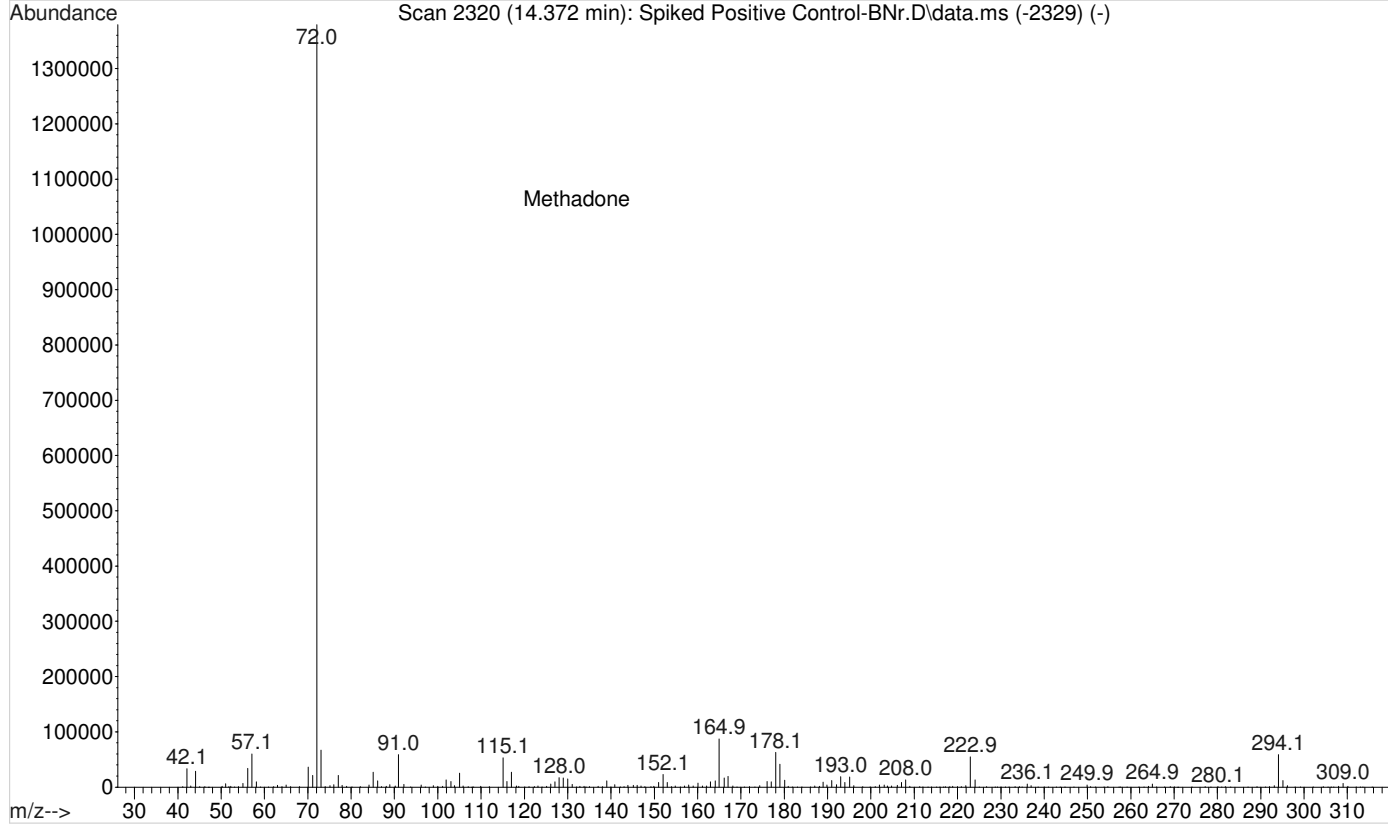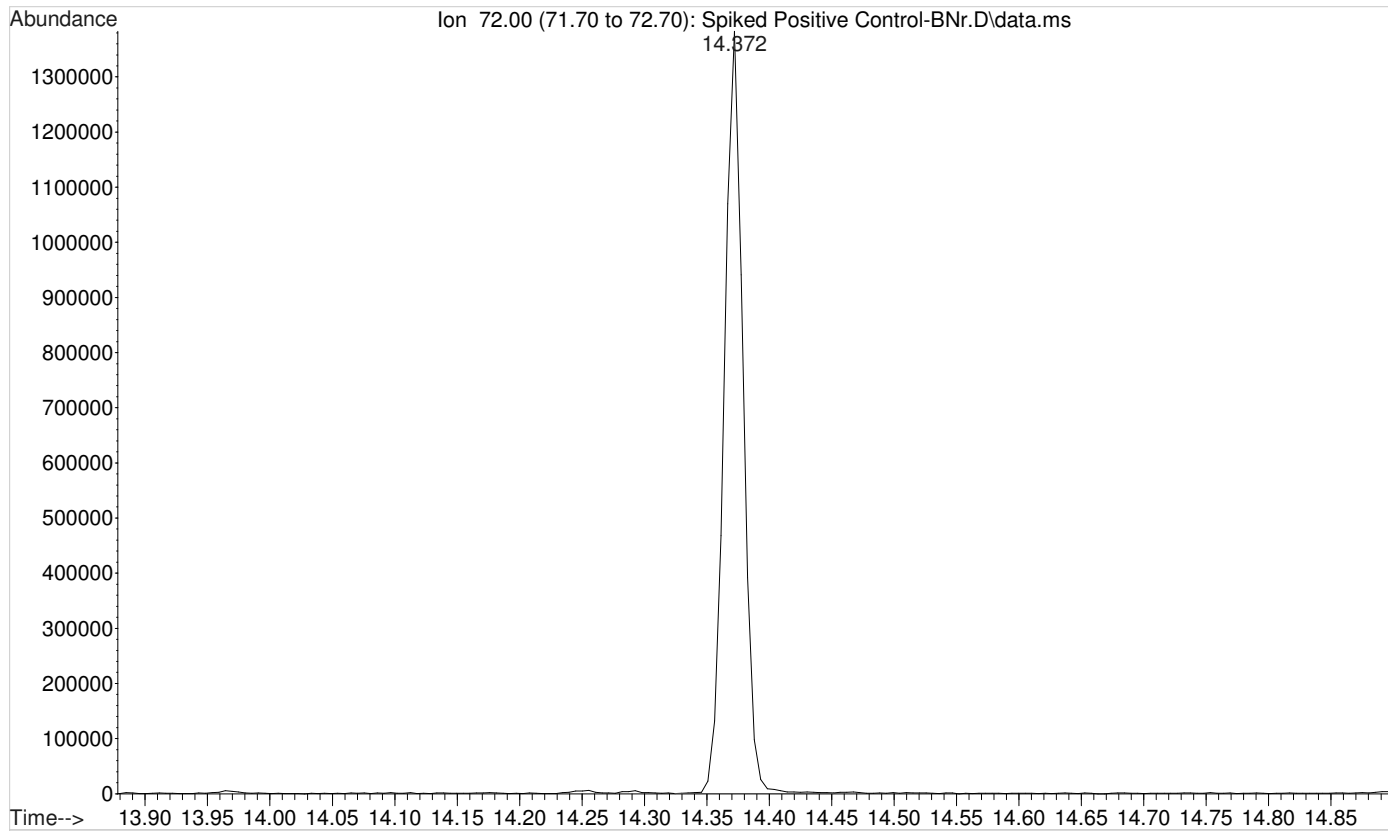



File :C:\MyFiles\cshrum\Desktop\101515 Data\Spiked Positive Control
... l-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 15 Oct 2015 22:15 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

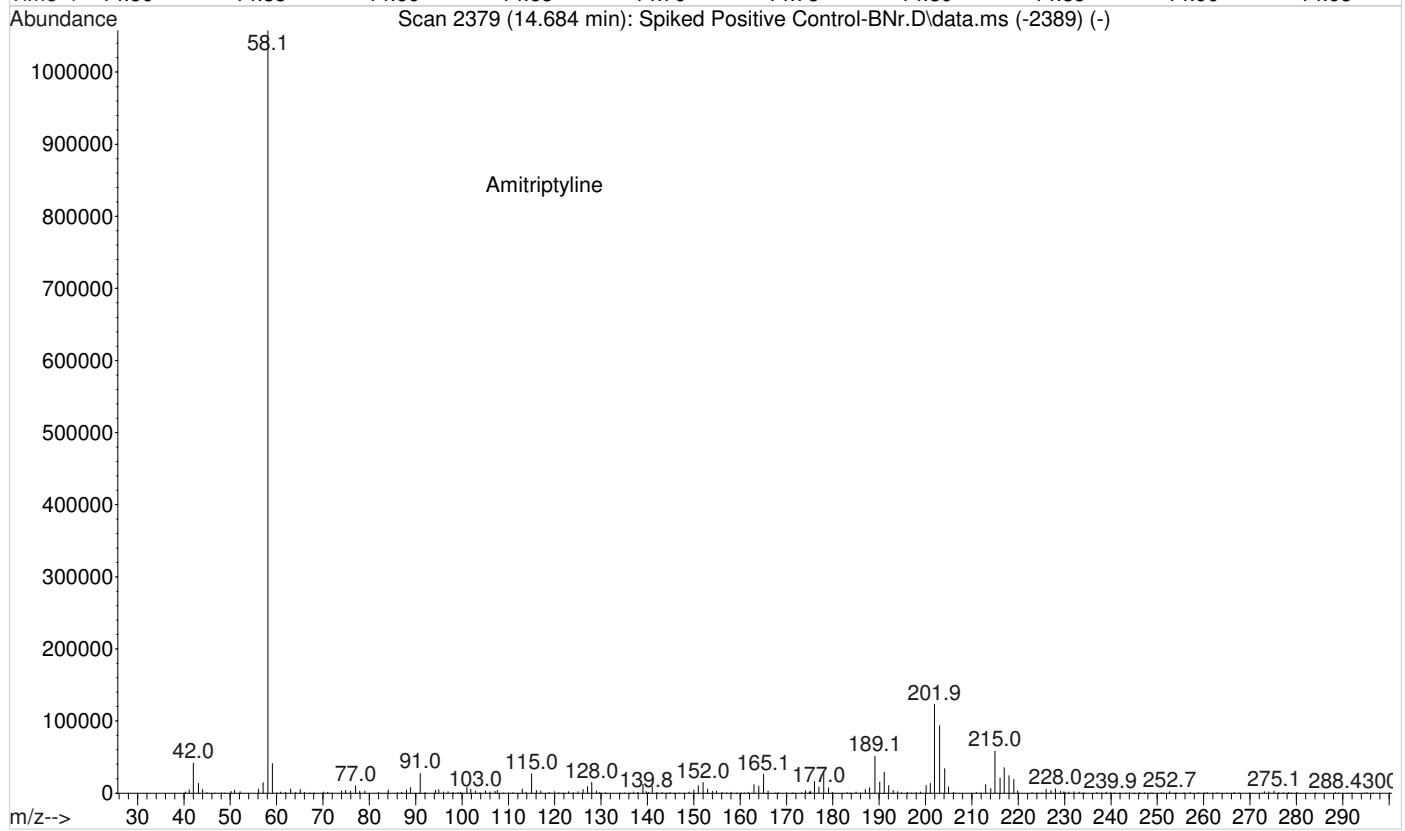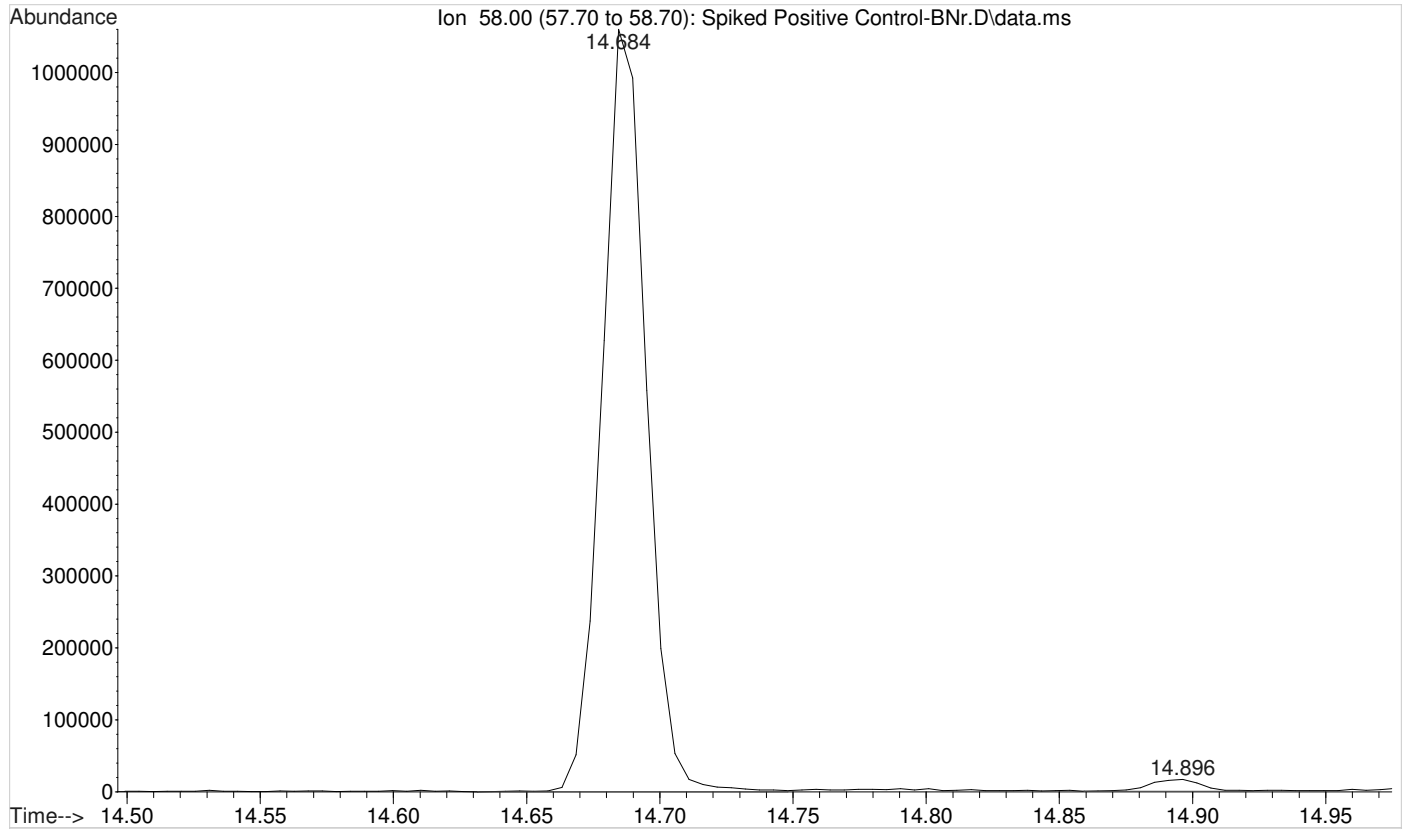



File :C:\MyFiles\cshrum\Desktop\101515 Data\Spiked Positive Control
... l-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 15 Oct 2015 22:15 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

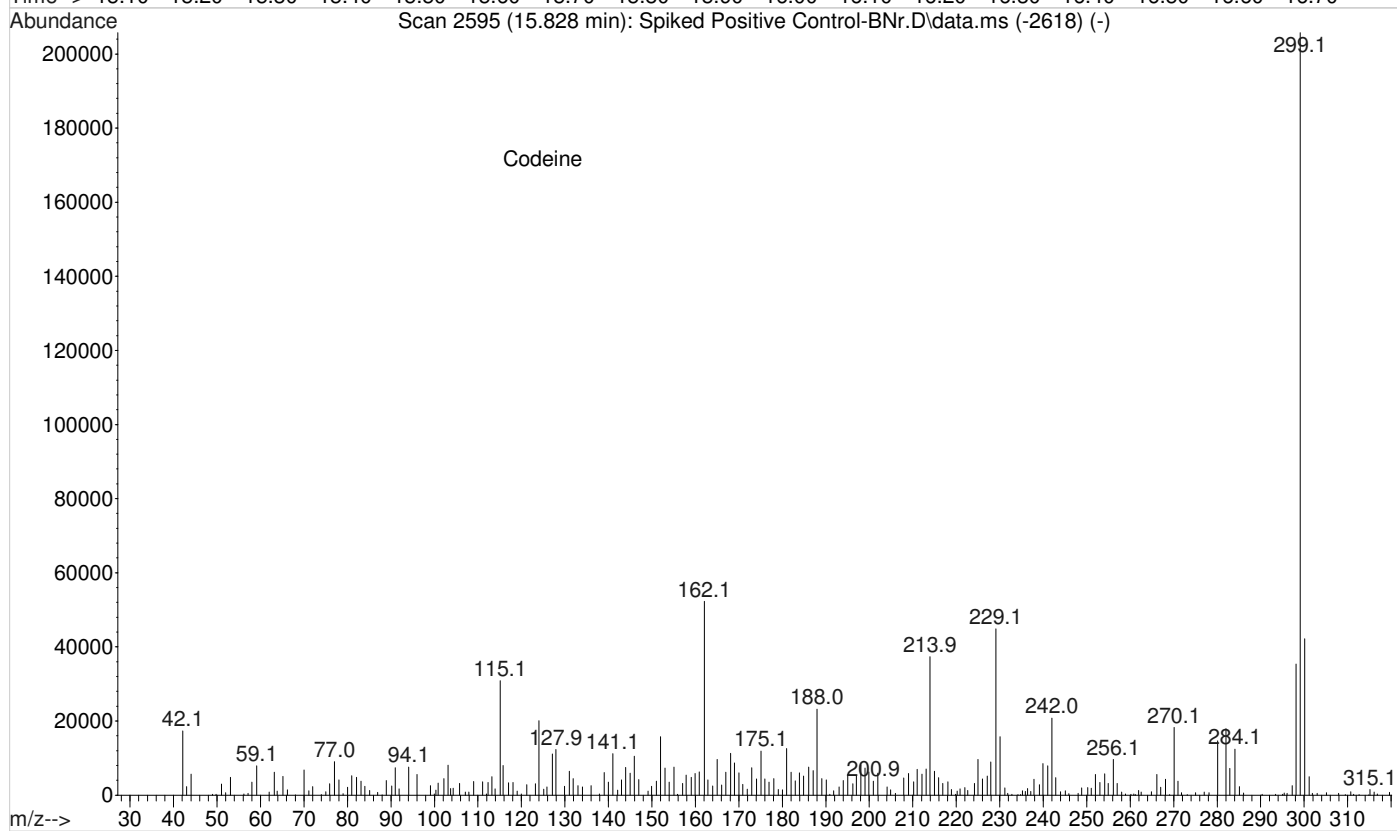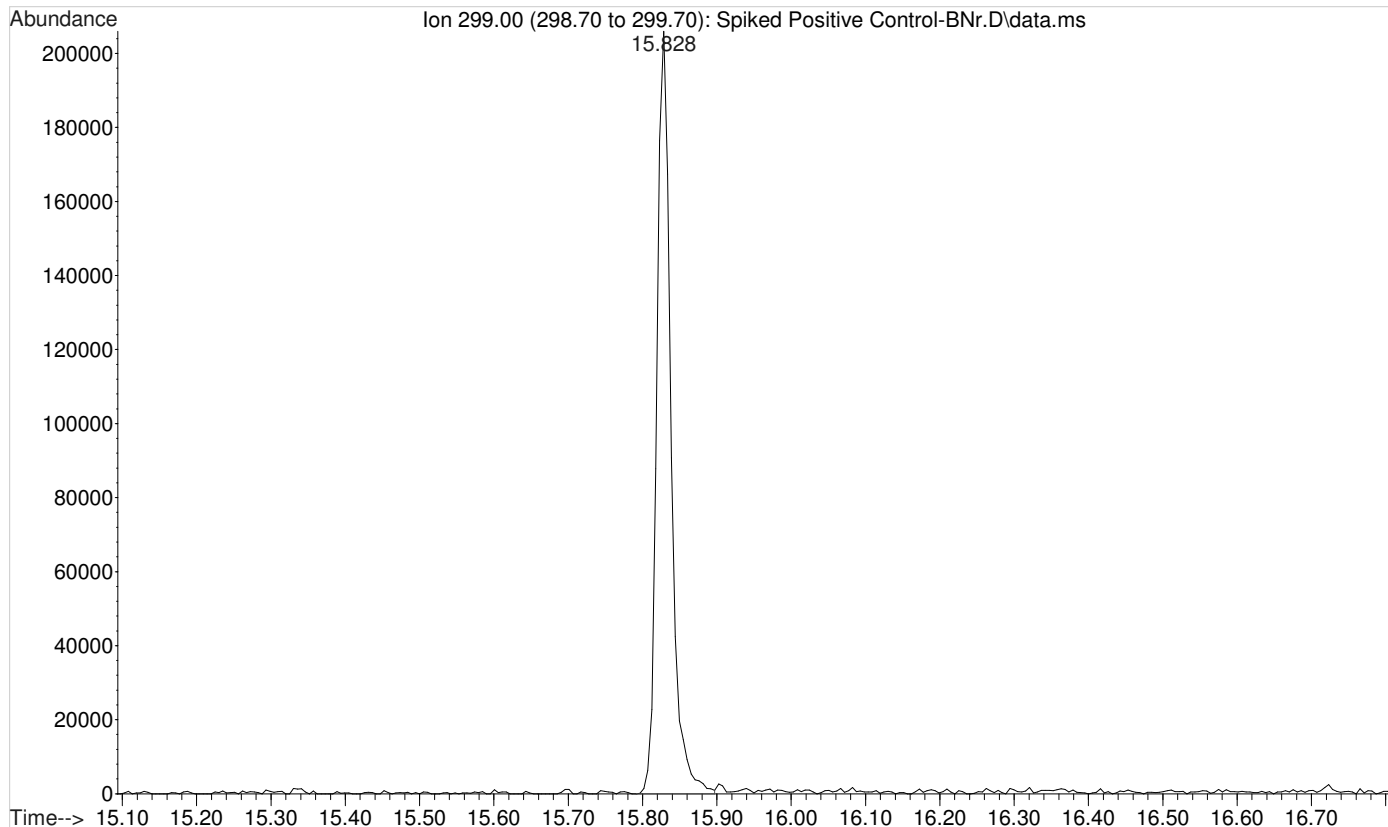



File :C:\MyFiles\cshrum\Desktop\101515 Data\Spiked Positive Contro
... l-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 15 Oct 2015 22:15 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

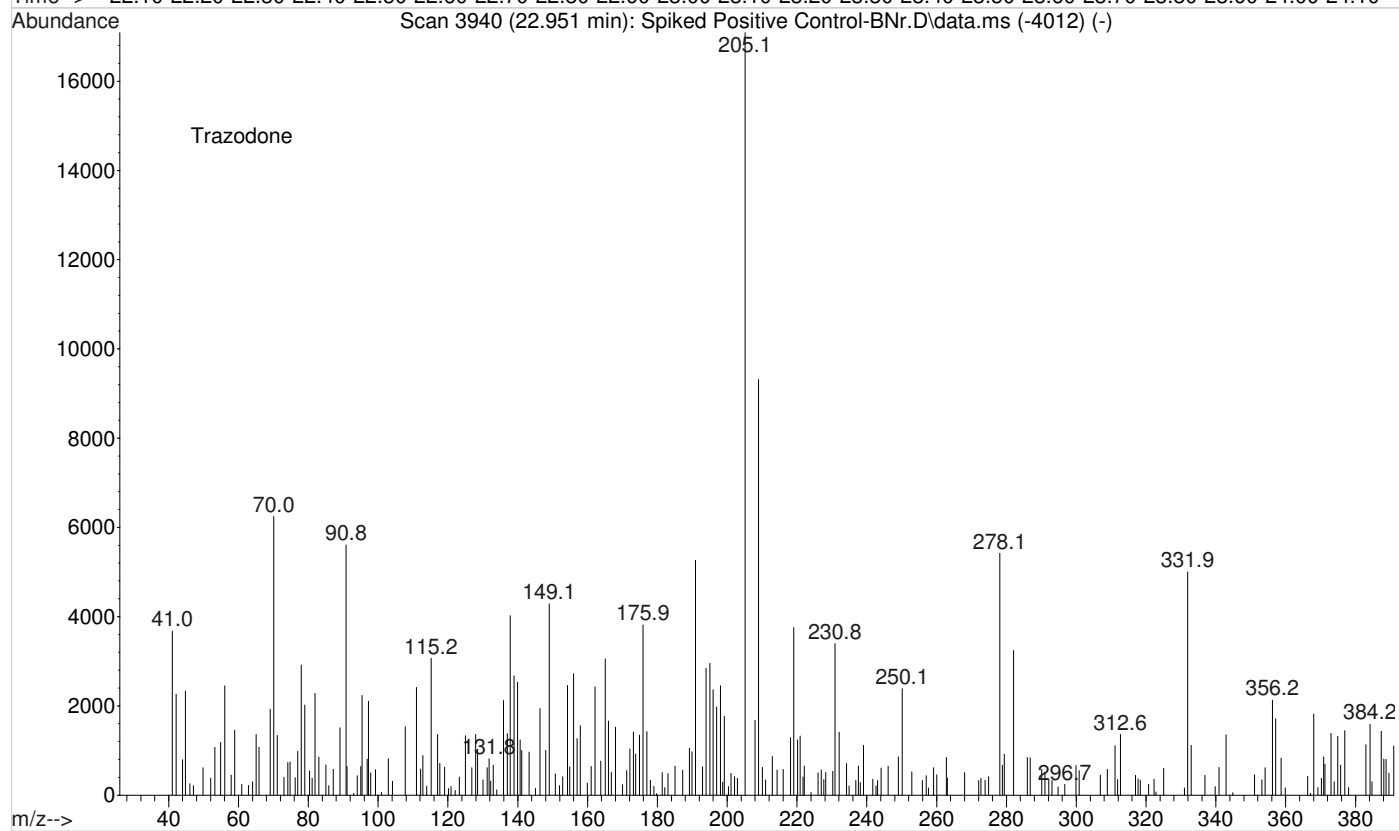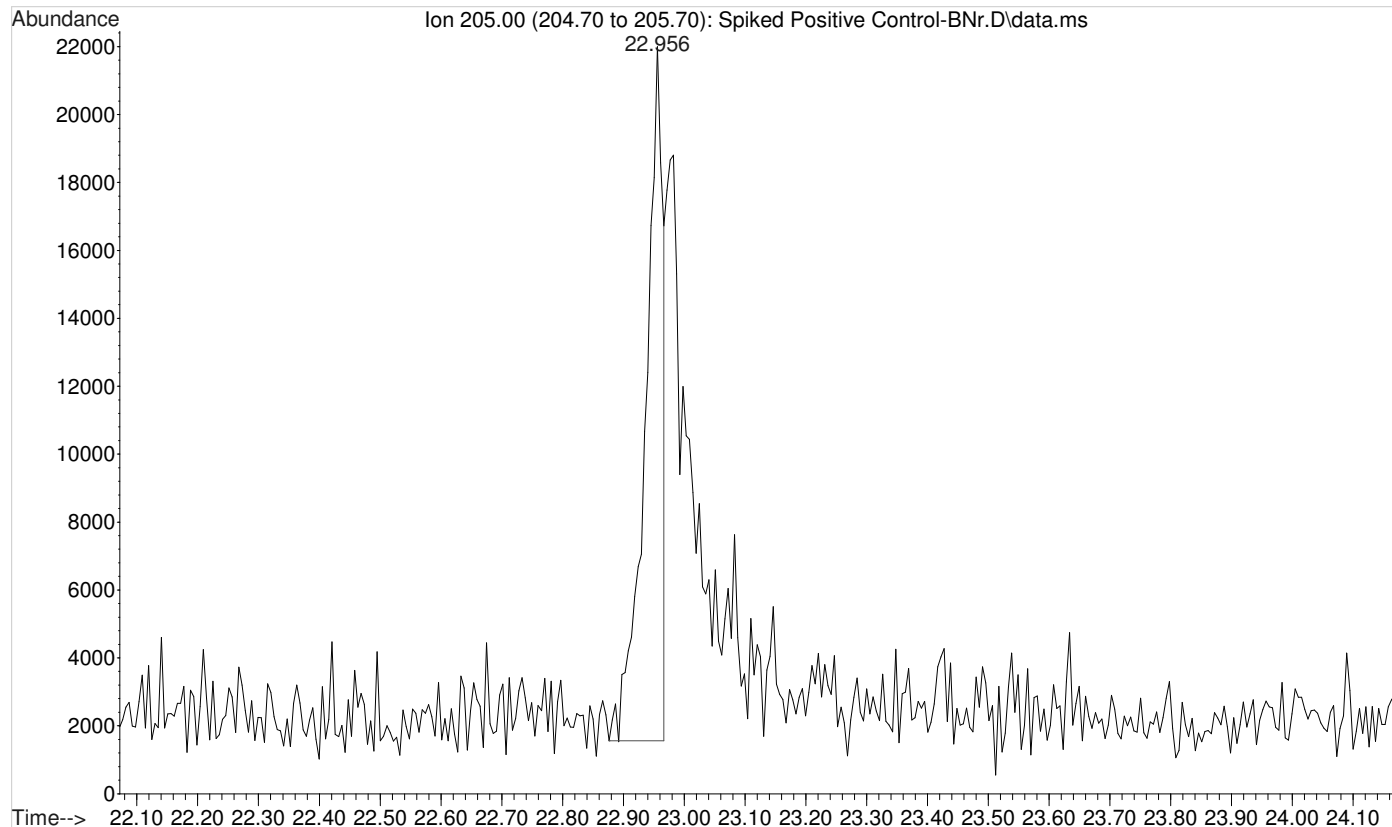



File :C:\MyFiles\cshrum\Desktop\101515 Data\Spiked Positive Control
... l-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 15 Oct 2015 22:15 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

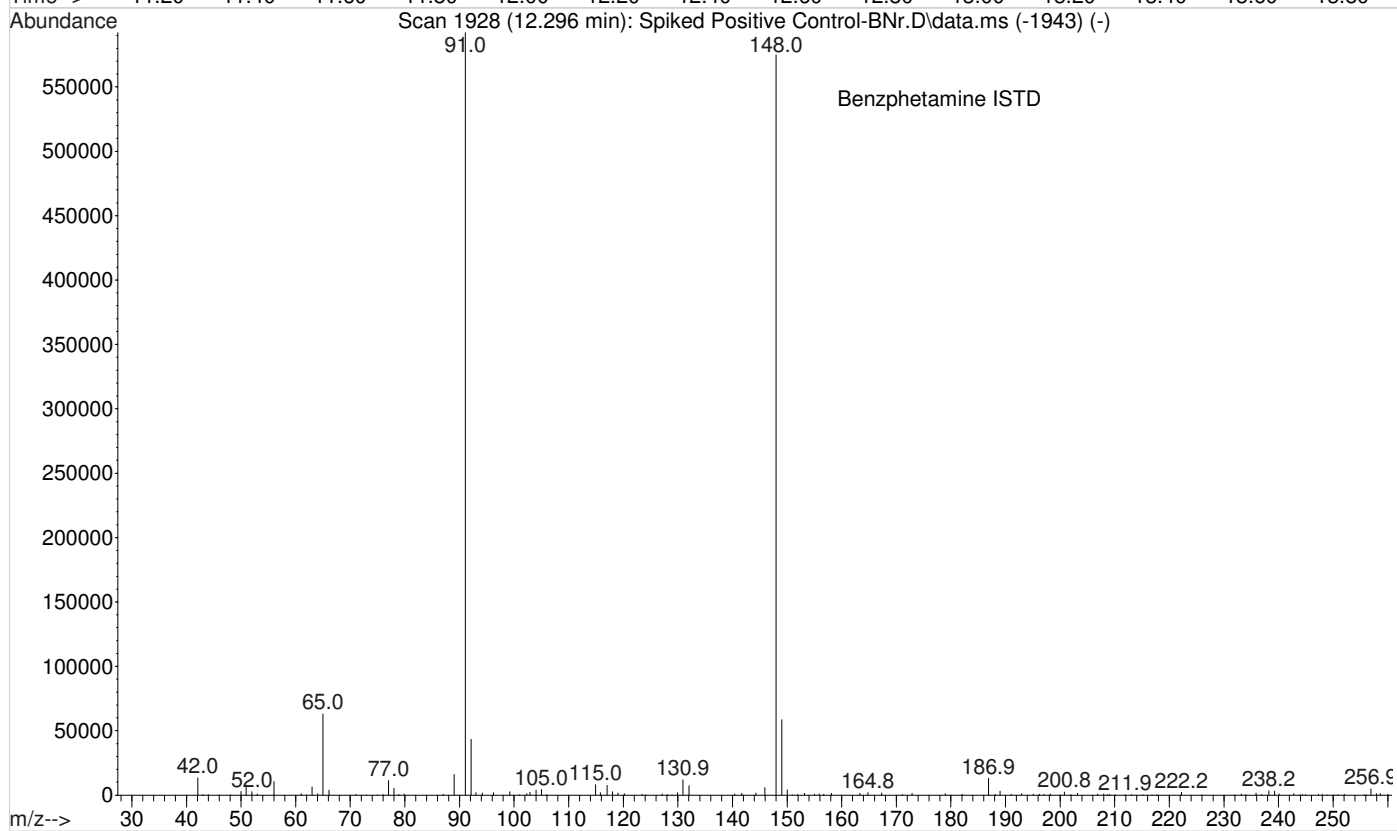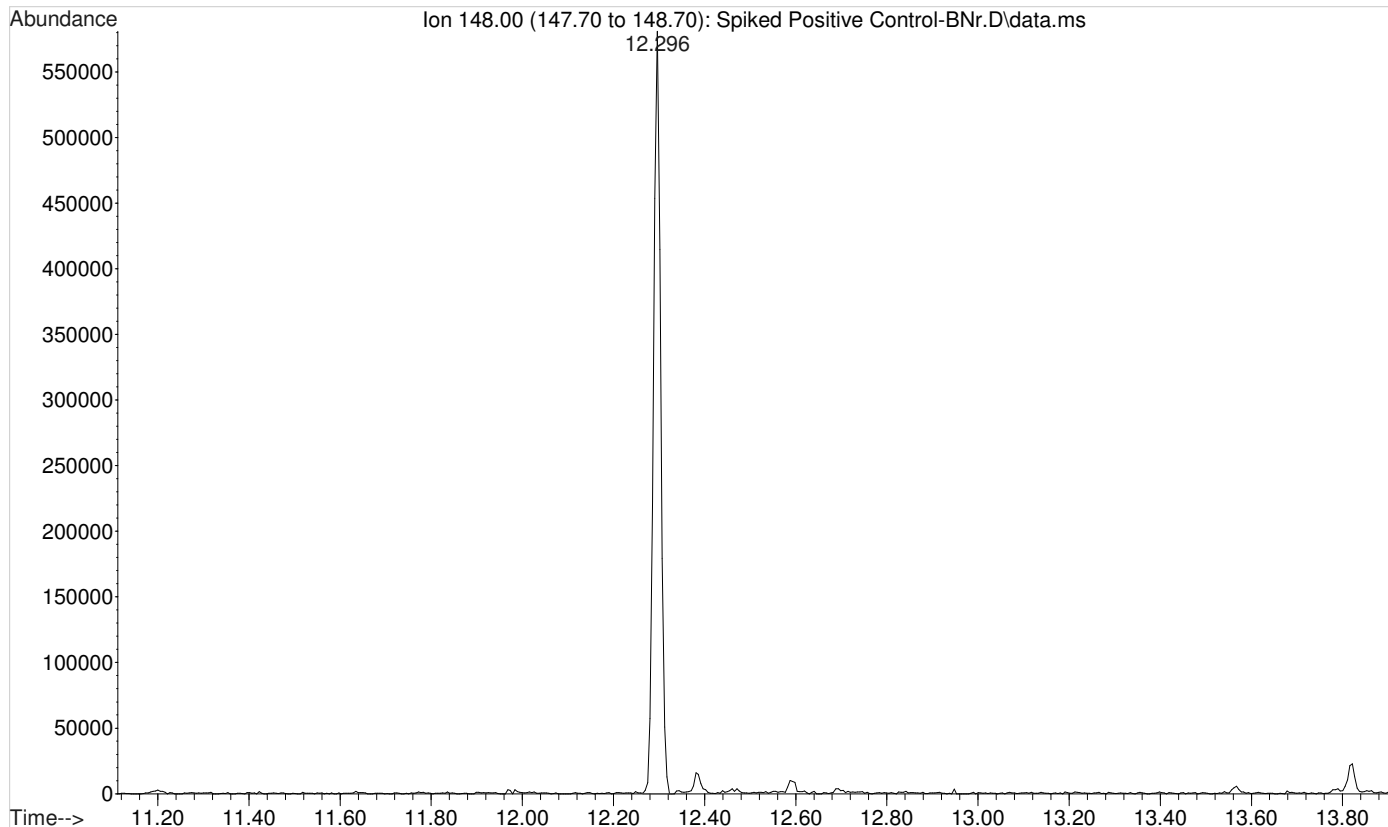



File :C:\MyFiles\cshrum\Desktop\101515 Data\Spiked Positive Contro
... l-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 15 Oct 2015 22:15 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

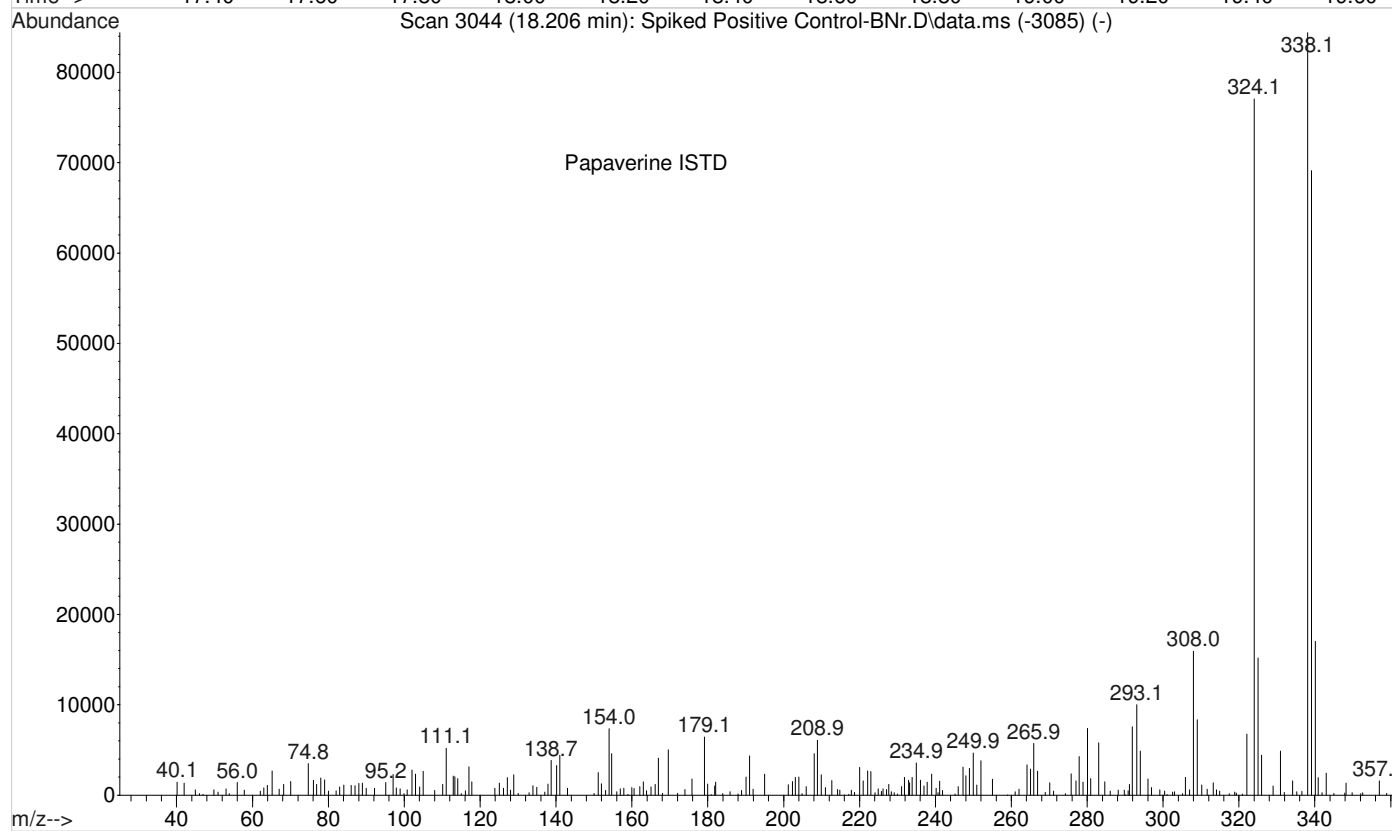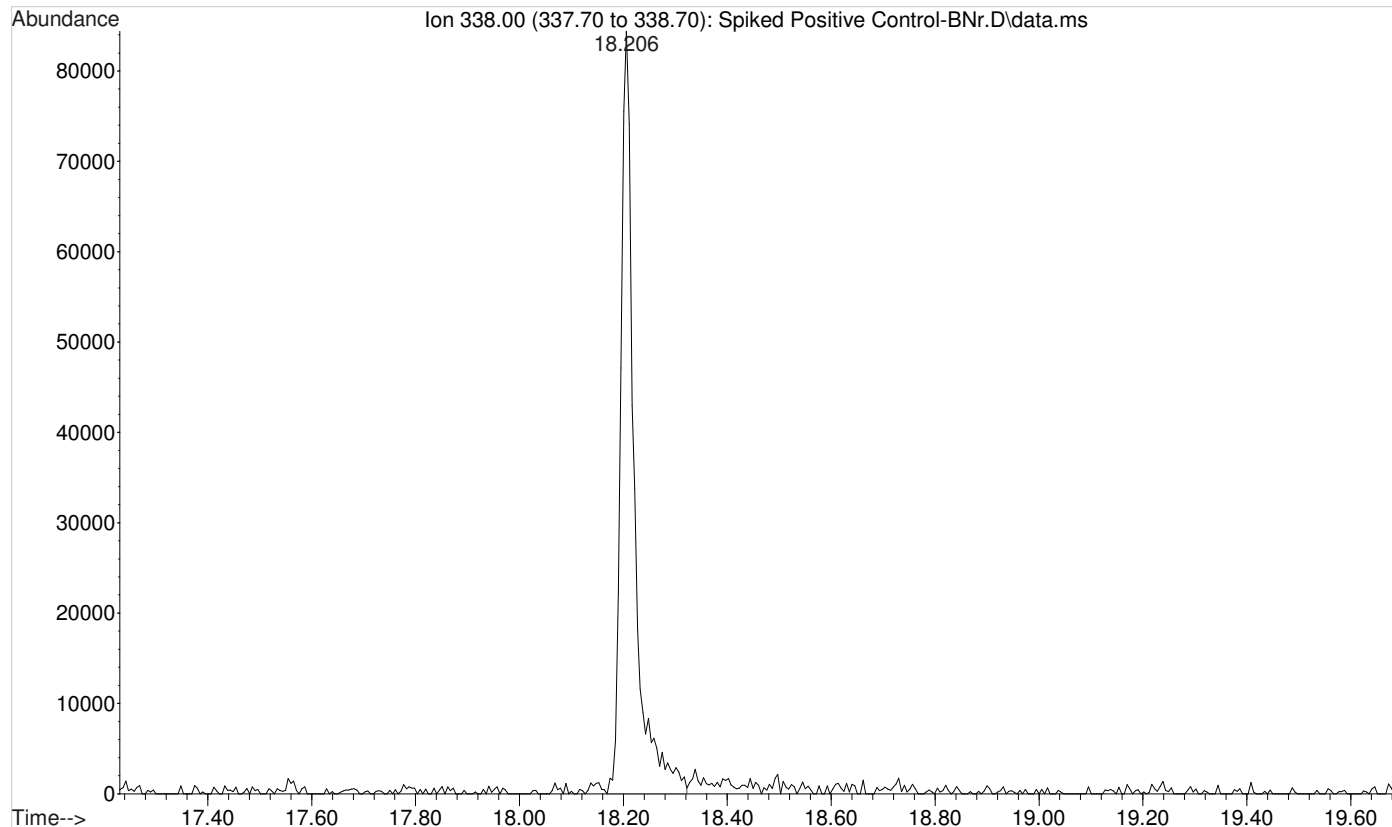



File :C:\MyFiles\cshrum\Desktop\101515 Data\Spiked Positive Control
... l-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 15 Oct 2015 22:15 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

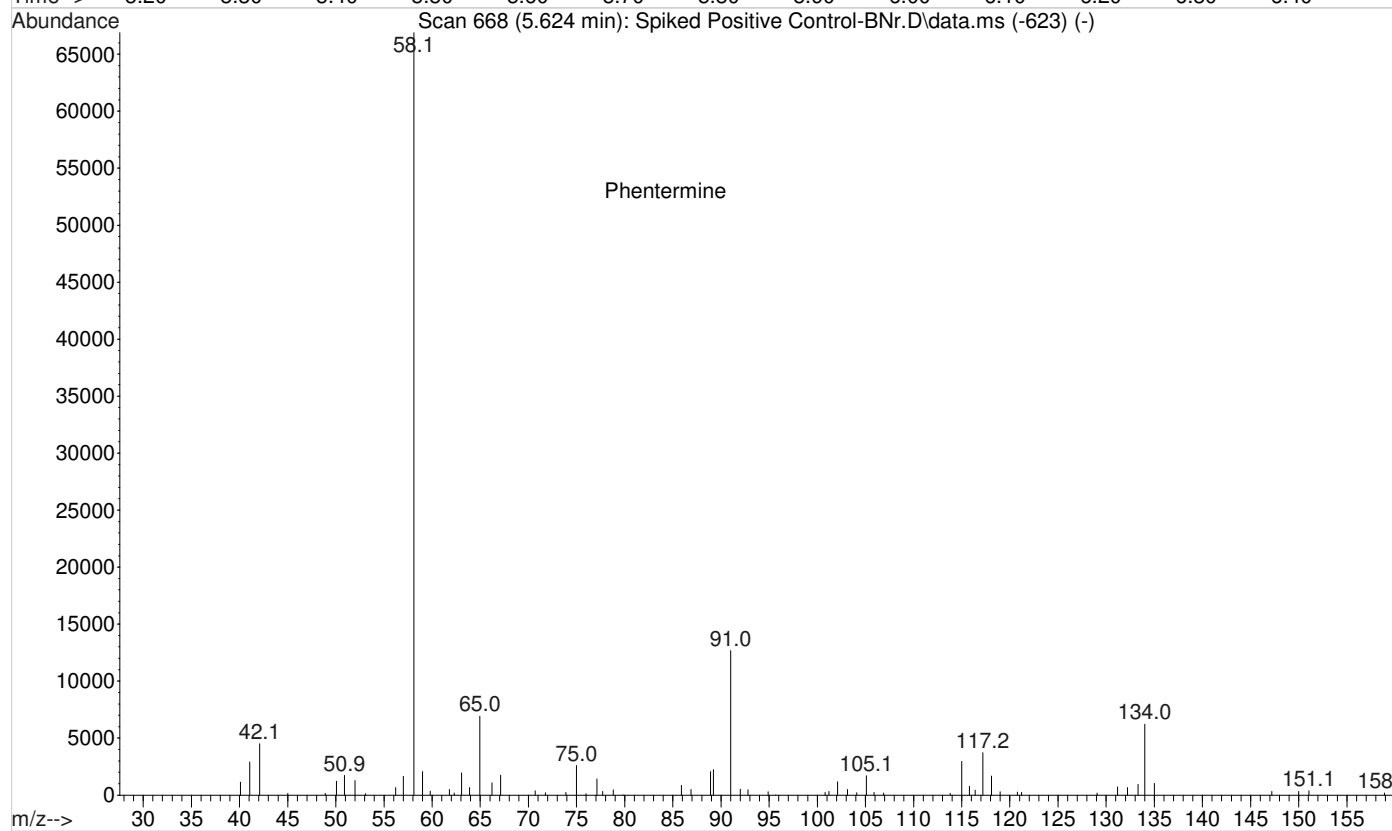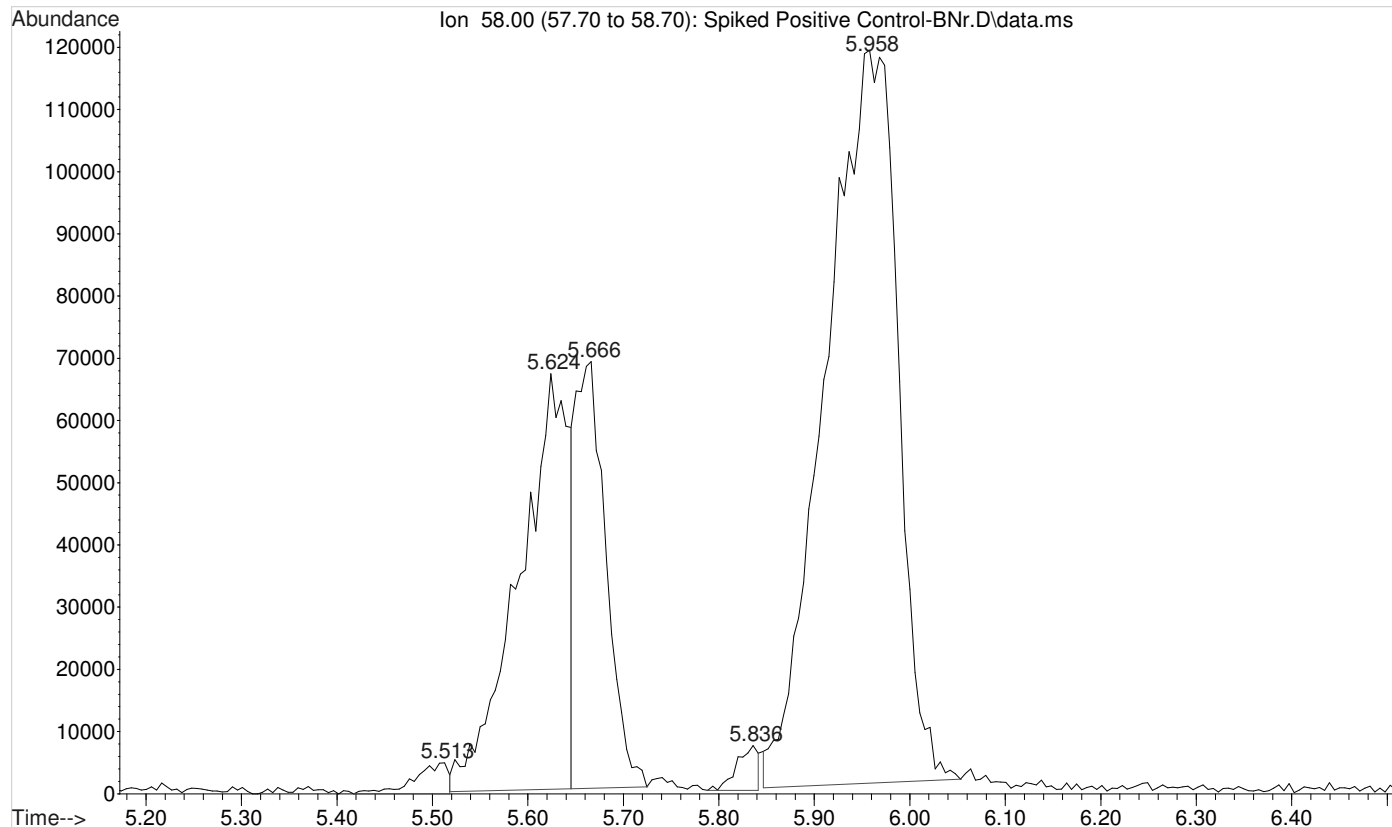



File :C:\MyFiles\cshrum\Desktop\101515 Data\Spiked Positive Control
... l-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 15 Oct 2015 22:15 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

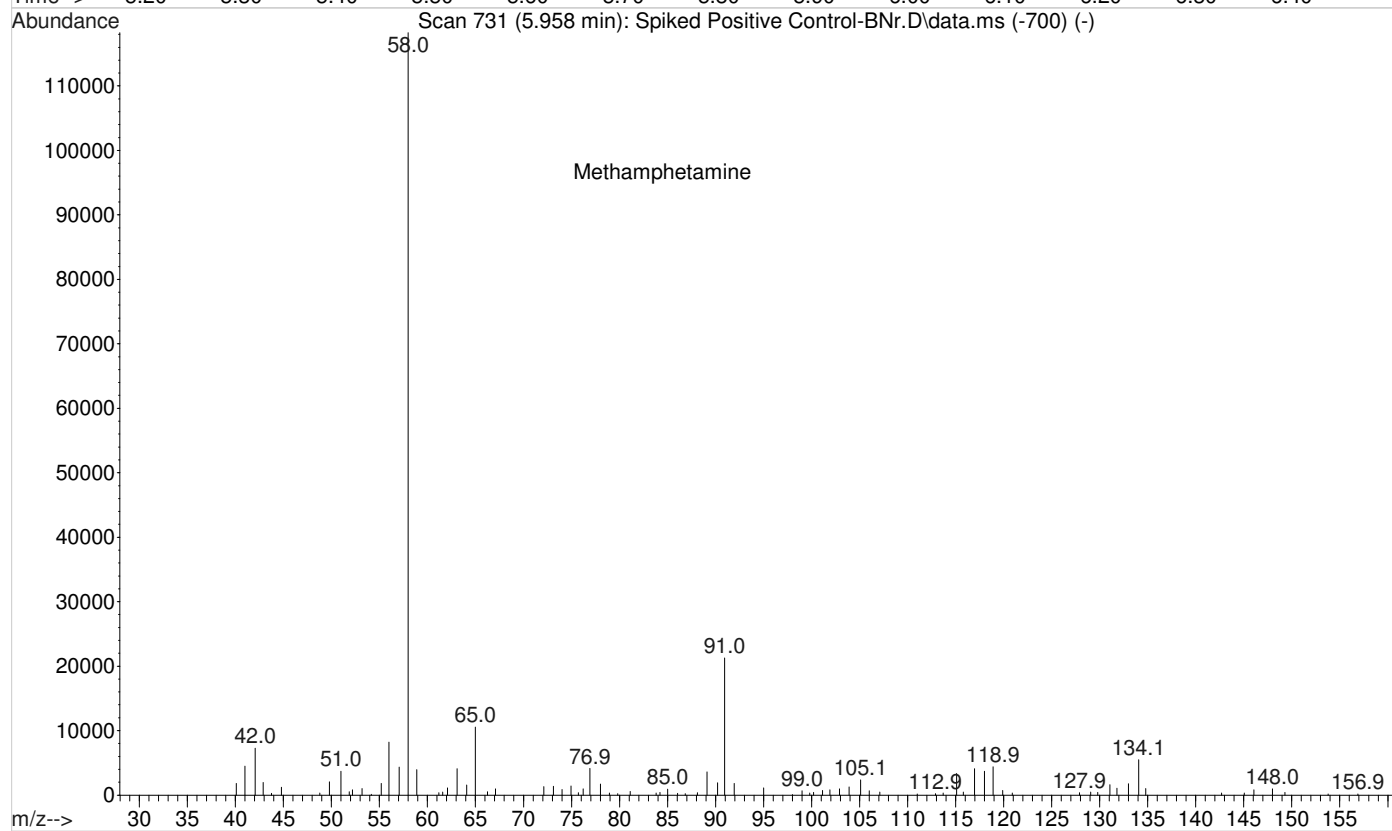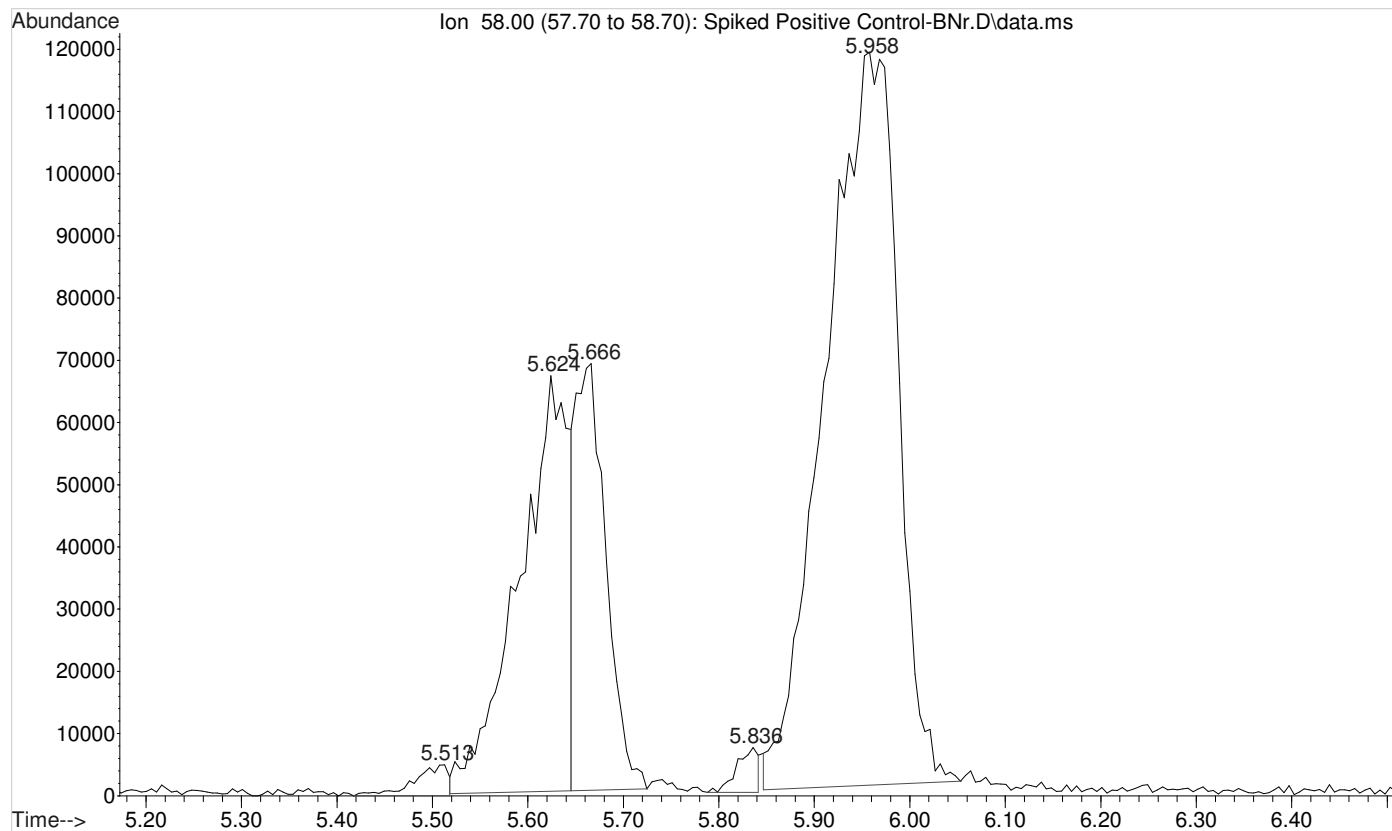



File :C:\MyFiles\cshrum\Desktop\101515 Data\Spiked Positive Control
... l-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 15 Oct 2015 22:15 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

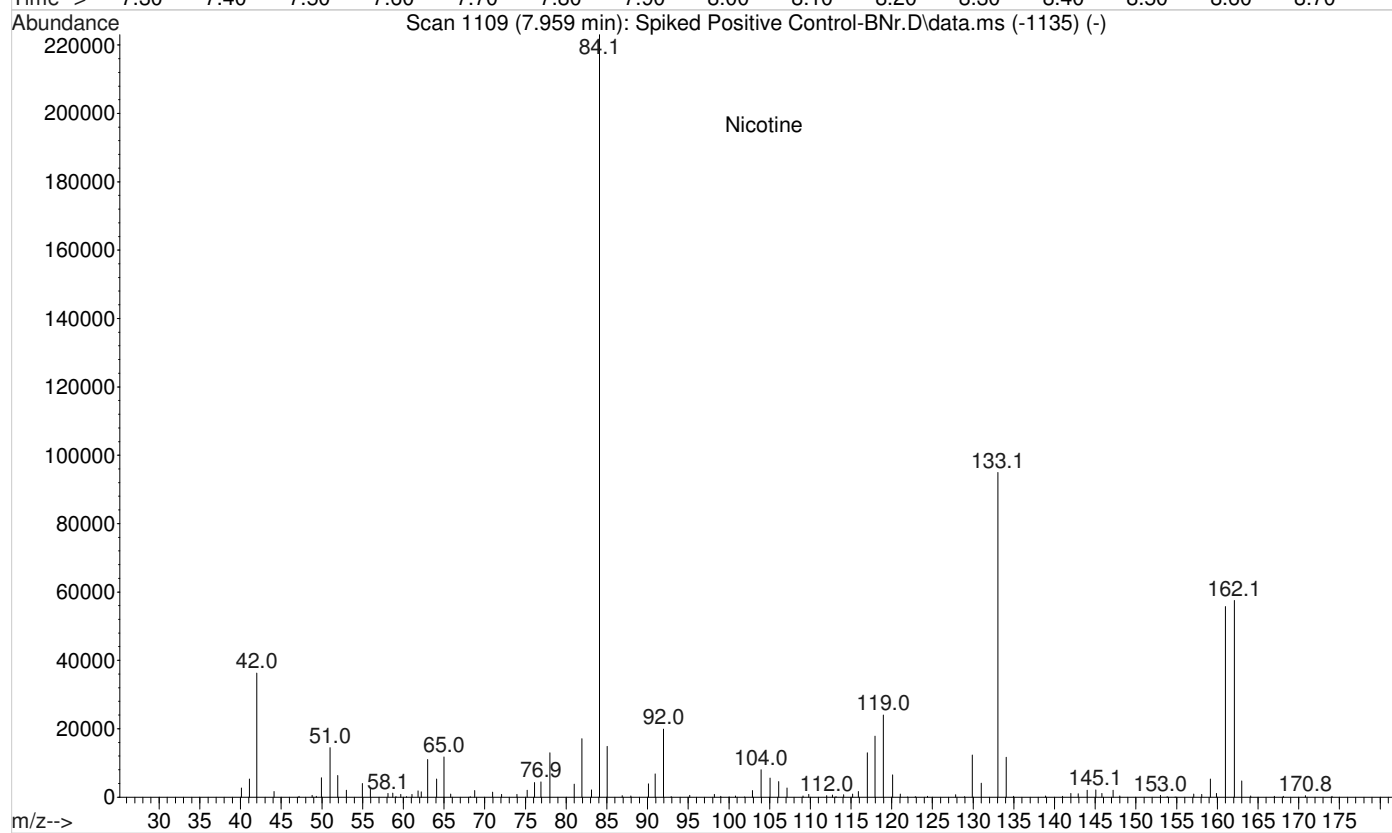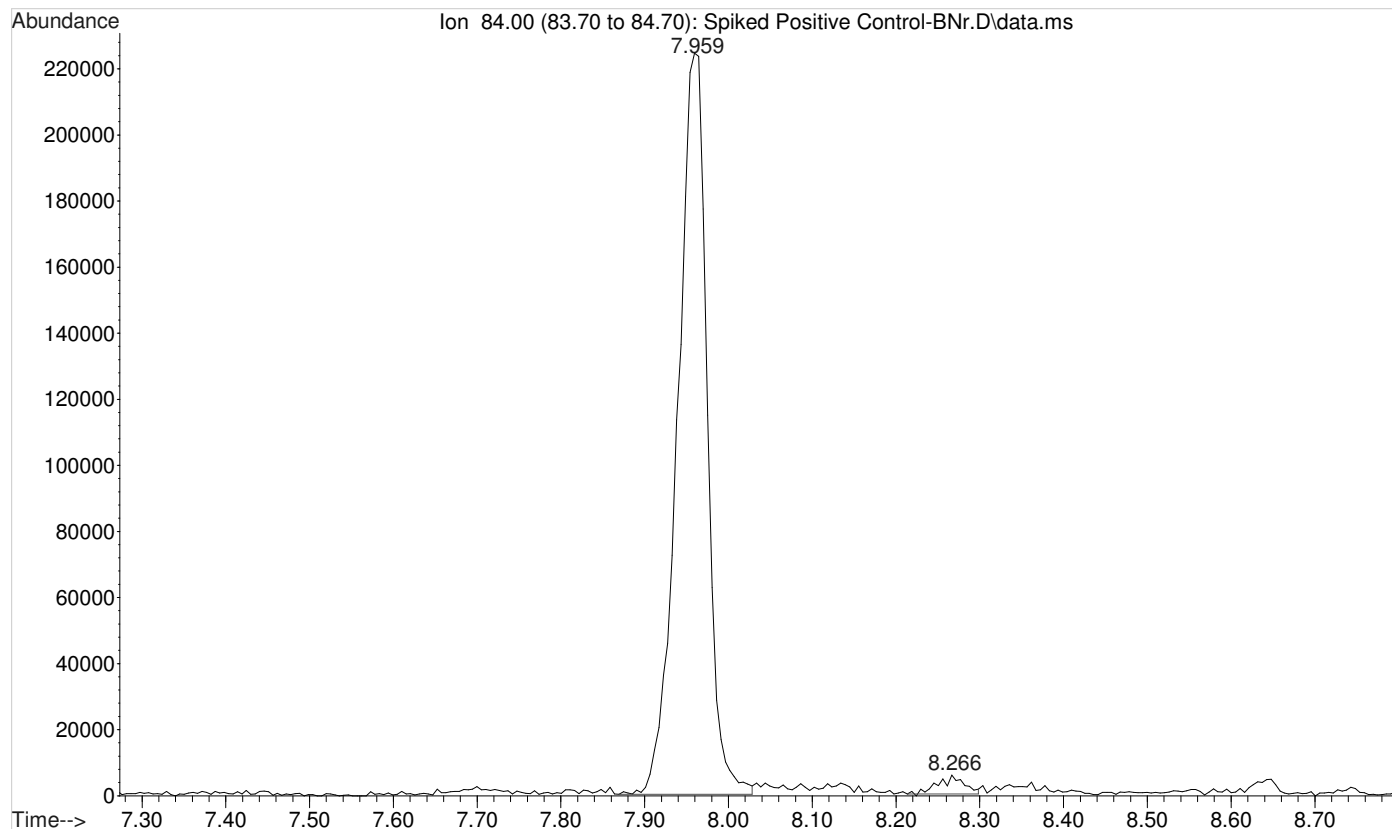



File :C:\MyFiles\cshrum\Desktop\101515 Data\Spiked Positive Control
... l-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 15 Oct 2015 22:15 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

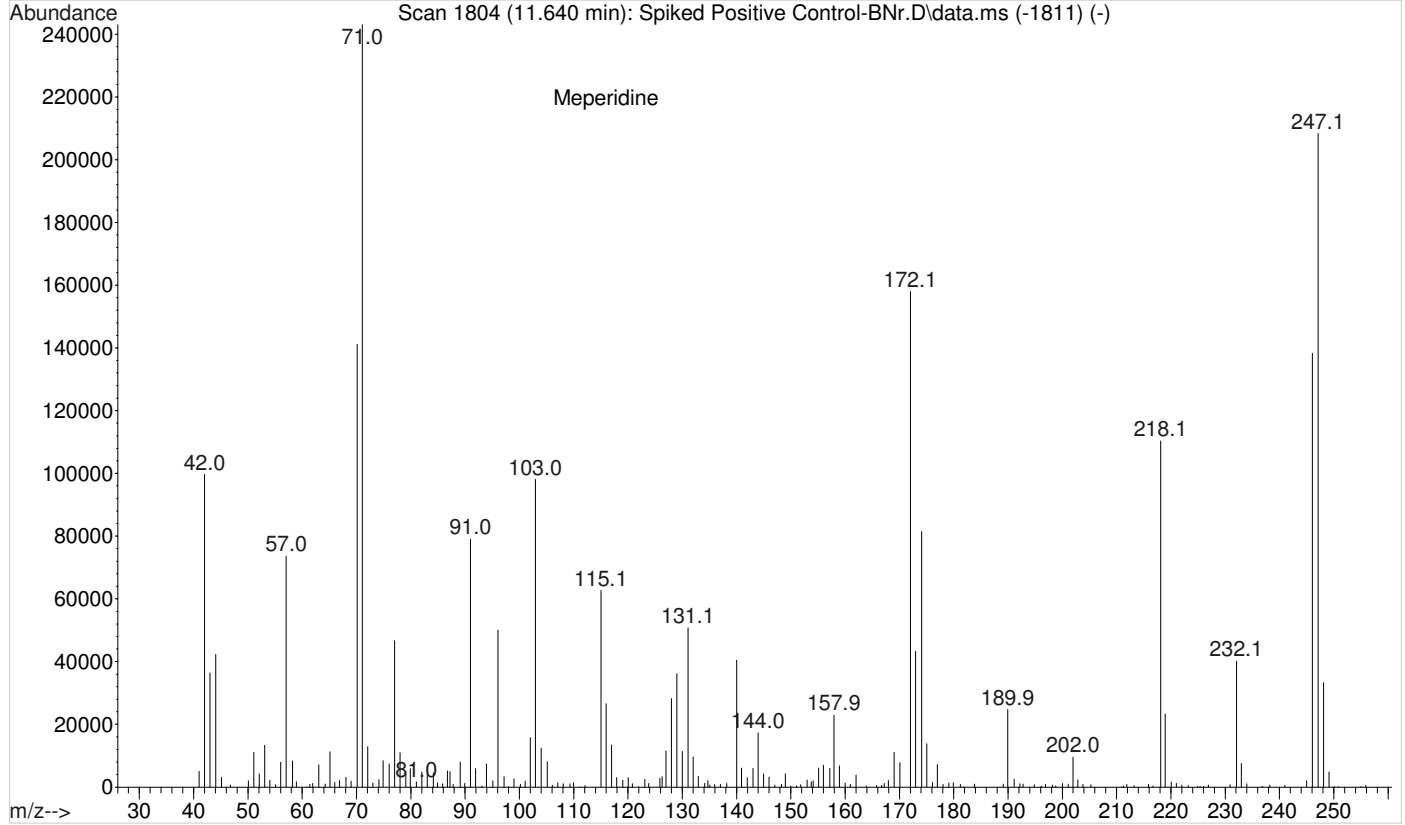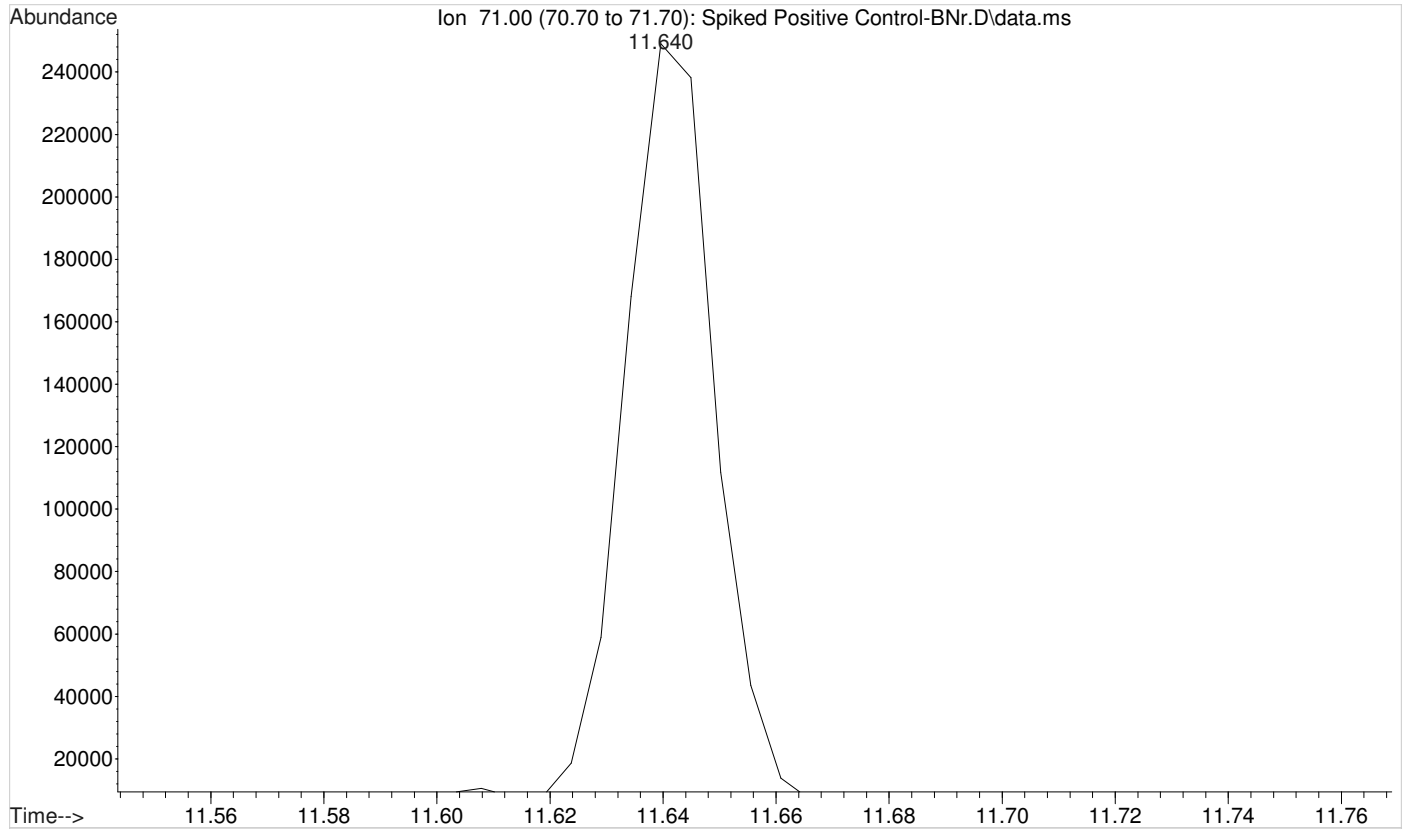



File :C:\MyFiles\cshrum\Desktop\101515 Data\Spiked Positive Contro
... l-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 15 Oct 2015 22:15 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

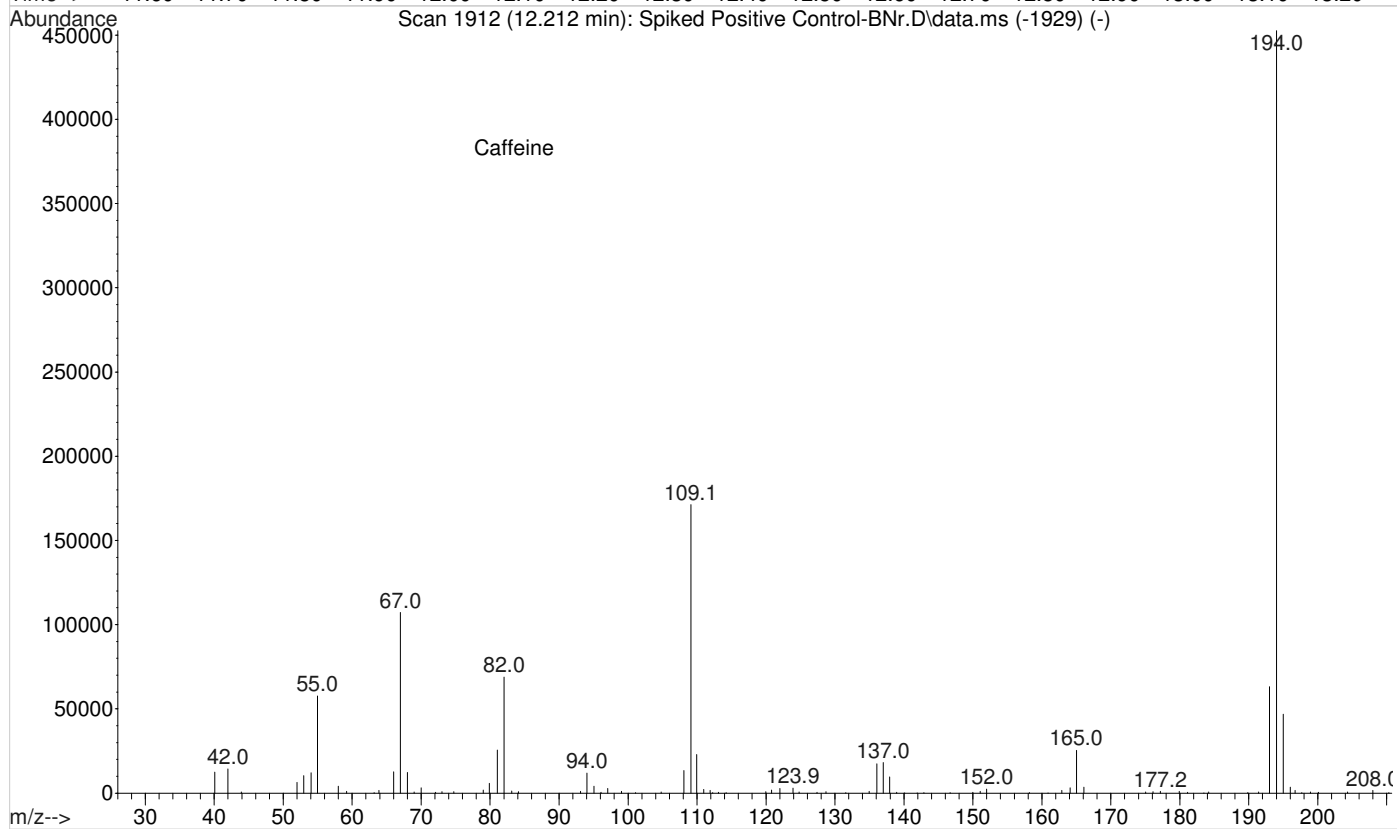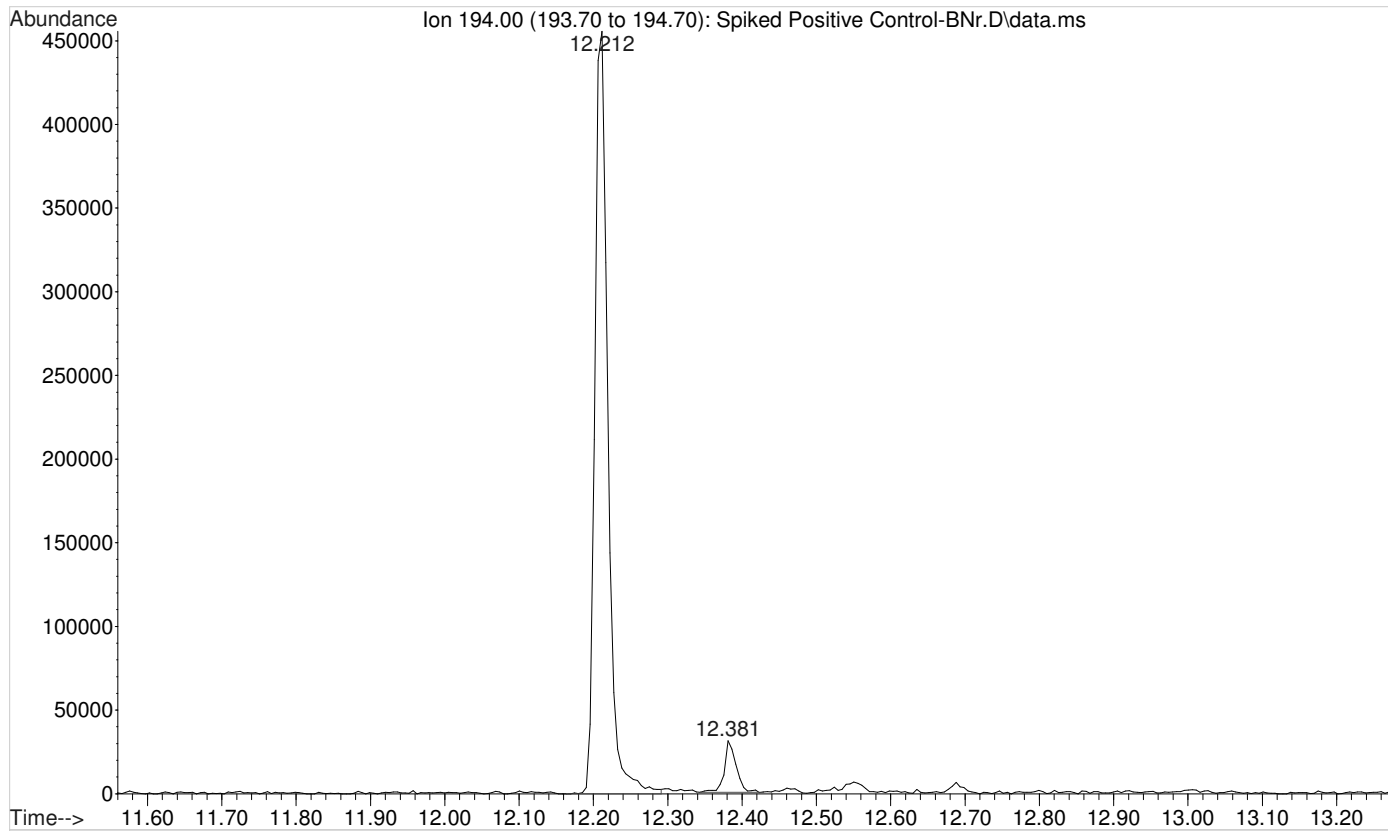

File :C:\MyFiles\cshrum\Desktop\101515 Data\Spiked Positive Control
... l-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 15 Oct 2015 22:15 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

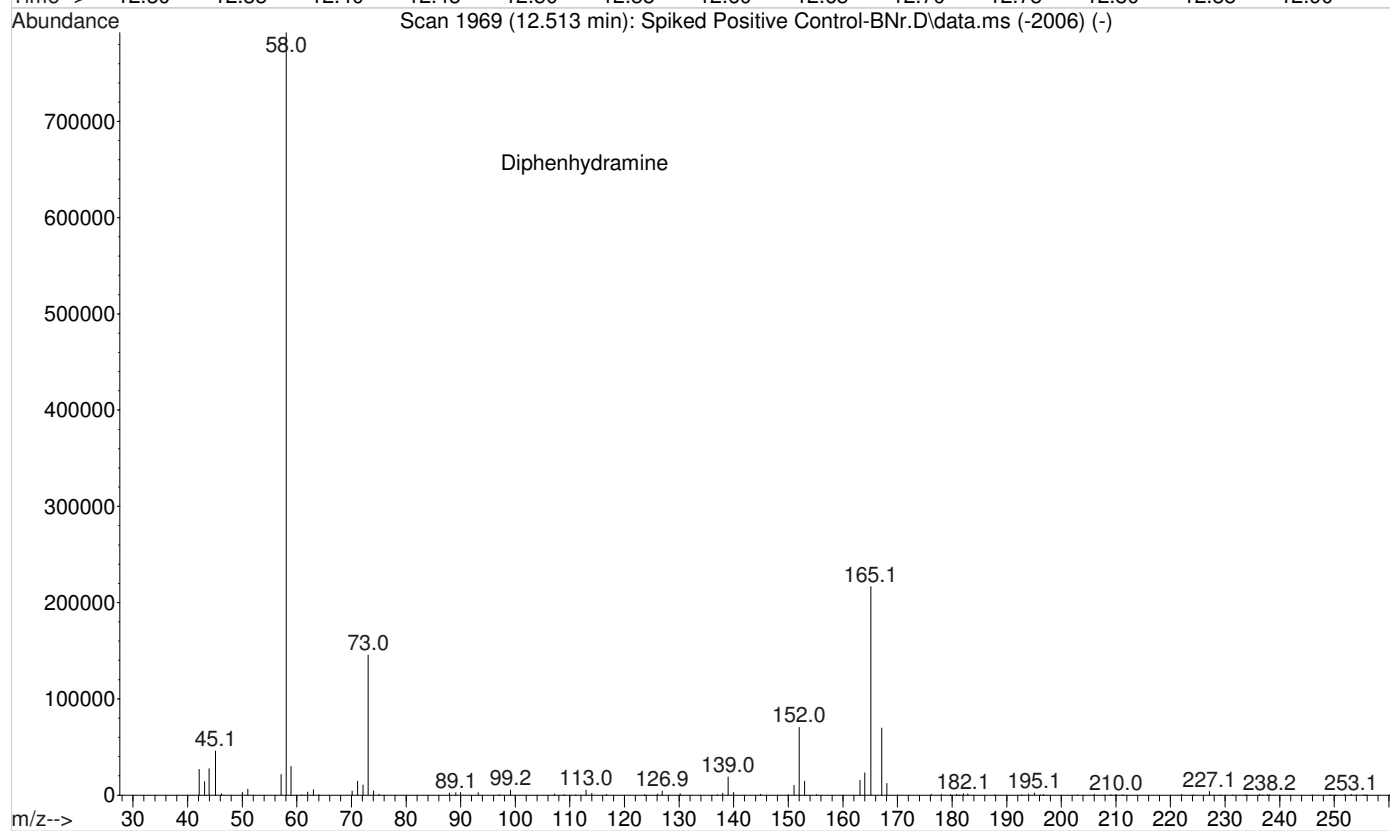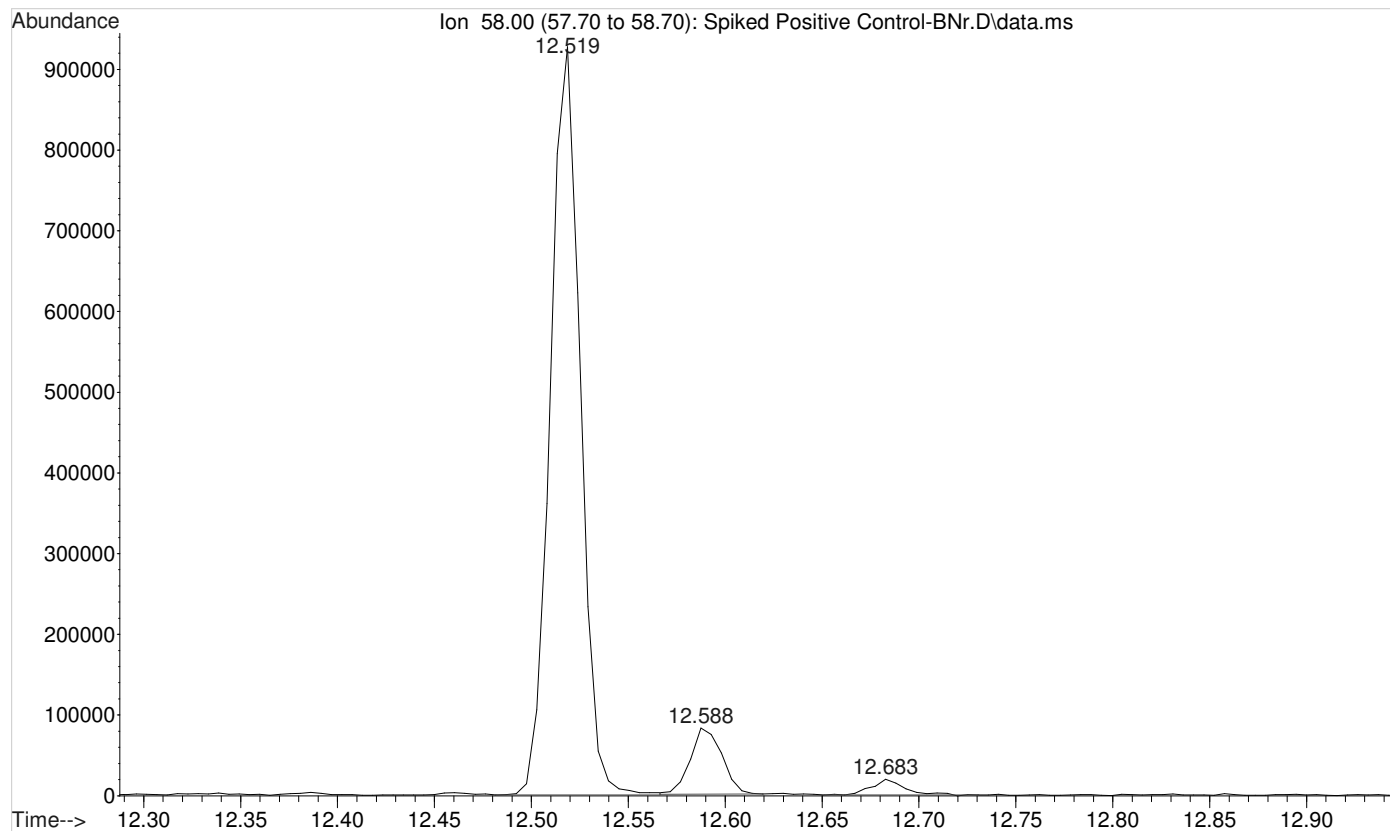

File :C:\MyFiles\cshrum\Desktop\101515 Data\prbLK2r.D
Operator : ISP\datastor
Acquired : 15 Oct 2015 22:50 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Solvent Blank
Misc Info : Chloroform
Vial Number: 99

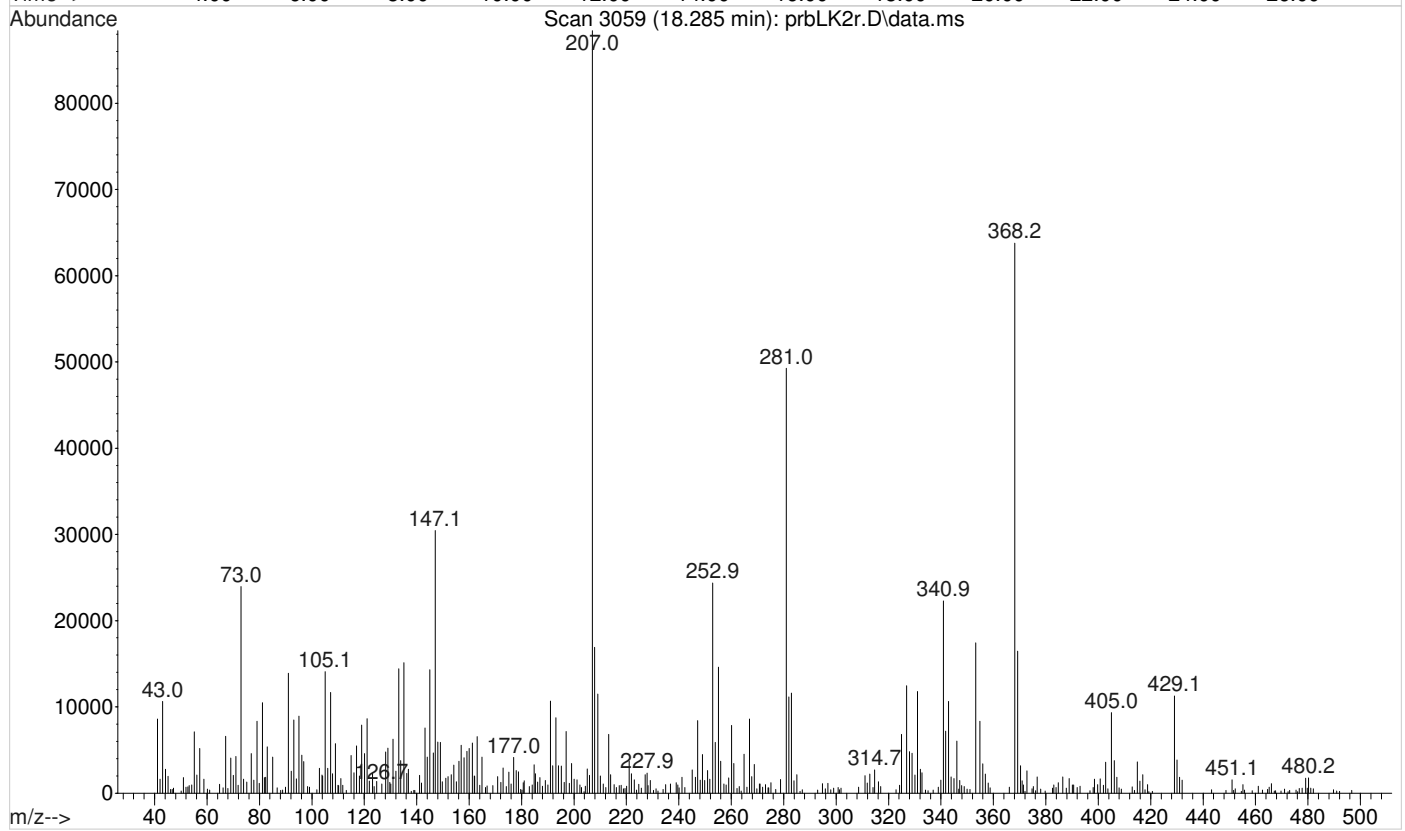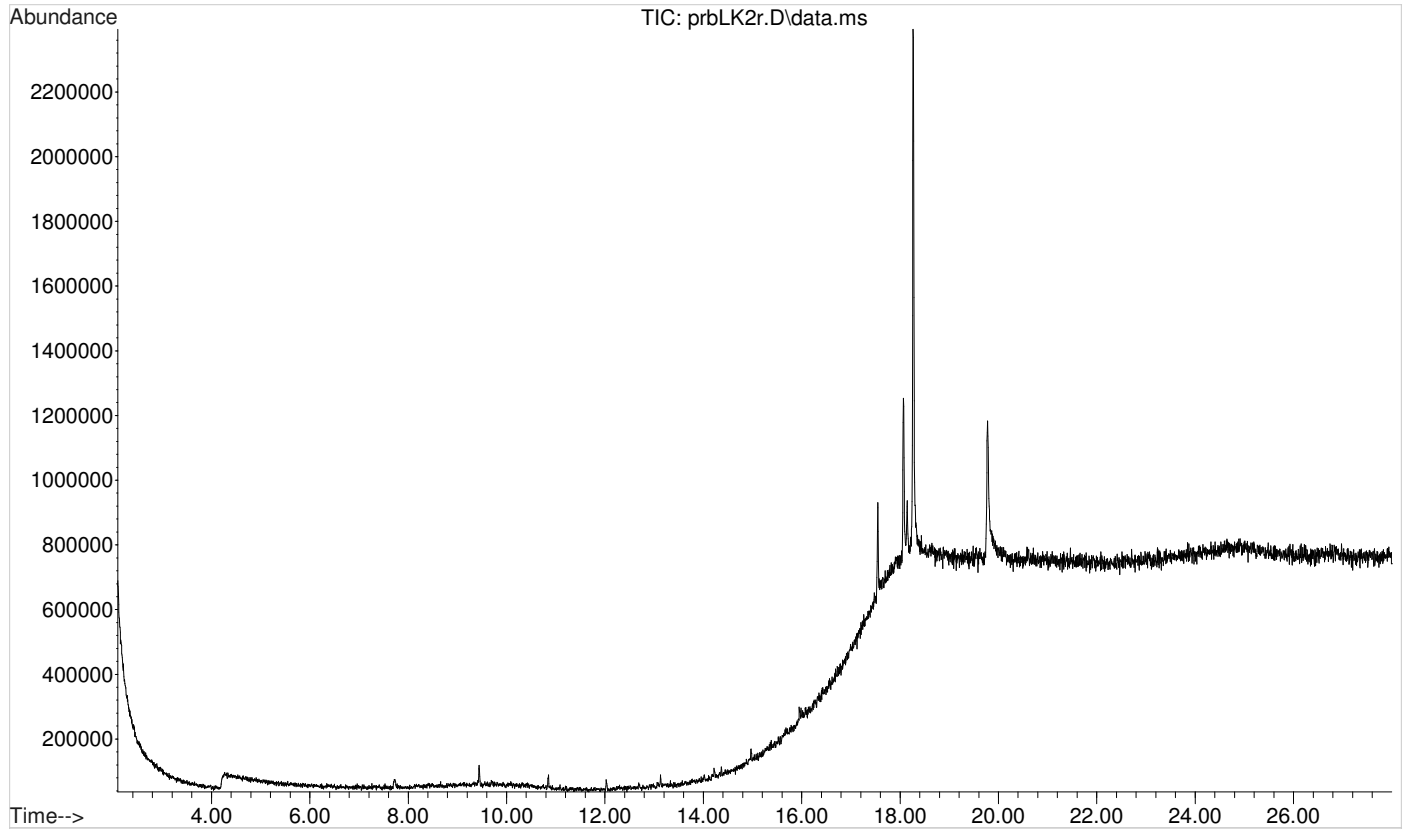

File :C:\MyFiles\cshrum\Desktop\101515 Data\AFTER.D
Operator : ISP\datastor
Acquired : 18 Oct 2015 00:31 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: BLK
Misc Info : Chloroform
Vial Number: 72

