

Quantitative Analysis for Ethanol & Qualitative Analysis for Other Volatiles

Analytical Method(s): 1.0

Device: Hamilton MICROLAB 503A Liquid Processor/Dilutor Serial Number: MD96BC1382/MD94AM10010

Volatiles Quality Assurance Controls

Run Dates: 11/17/17-11/18/17
Calibration: 11/09/17

Control level	Expiration	Lot #	Target Value	Acceptable Range	Overall Results
Level 1	Jul-18	1407031	0.0780	0.0702-0.0858	0.0776 g/100cc 0.0825 g/100cc g/100cc
Level 2	Jul-18	1407032	0.2020	0.1818-.2222	0.1998 g/100cc 0.2065 g/100cc g/100cc
Multi-Component mixture:		Exp date: Oct 2019	Lot #	FN09231404	OK
Curve Fit:		Column 1	Column 2	0.99999	0.99994

Ethanol Calibration Reference Material		
Calibrator level	Expiration	Cerilliant Lot #
0.050	Jul-19	FN06231406
0.080		
0.100	Jun-19	FN06181501
0.200	Dec-19	FN12011401
0.300	Feb-21	FN02121601
0.400		
0.500	Aug-19	FN07031402

	Target Value	Acceptable Range	Column 1	Column 2	Precision	Mean
	0.050	0.045 - 0.055	0.0506	0.0525	0.0019	0.0515
	0.080	0.072 - 0.088			0	#DIV/0!
	0.100	0.090 - 0.110	0.1000	0.0995	0.0005	0.0997
	0.200	0.180 - 0.220	0.1989	0.1974	0.0015	0.1981
	0.300	0.270 - 0.330	0.3003	0.2991	0.0012	0.2997
	0.400	0.360 - 0.440			0	#DIV/0!
	0.500	0.450 - 0.550	0.5002	0.5014	0.0012	0.5008

Aqueous Controls		
Control level	Expiration	Cerilliant Lot #
0.080	Nov-20	FN10281510

Target Value	Acceptable Range	Overall Results
0.08000	0.076 - 0.084	0.08 g/100cc

Issued: 4/22/2015
























~Any information on this document can be changed for laboratory use, except for the precision and mean determination formulas.

Volatiles QA/QC data spreadsheet Rev 5

Issuing Authority: Quality Manager

20

Worklist: 2036

<u>LAB CASE</u>	<u>ITEM</u>	<u>TASK ID</u>	<u>DESCRIPTION</u>	
M2017-5087	1	99165	Alcohol Analysis	
M2017-5088	1	99166	Alcohol Analysis	
M2017-5089	2	99175	Alcohol Analysis	
M2017-5090	1	99182	Alcohol Analysis	
M2017-5145	1	99423	Alcohol Analysis	
M2017-5154	1	99460	Alcohol Analysis	
M2017-5155	1	99461	Alcohol Analysis	
M2017-5158	1	99526	Alcohol Analysis	
M2017-5159	1	99527	Alcohol Analysis	
M2017-5160	1	99530	Alcohol Analysis	
M2017-5180	1	99557	Alcohol Analysis	
M2017-5190	1	99609	Alcohol Analysis	
M2017-5194	1	99624	Alcohol Analysis	
M2017-5196	2	99638	Alcohol Analysis	
M2017-5203	1	99659	Alcohol Analysis	
M2017-5204	1	99662	Alcohol Analysis	
M2017-5205	1	99663	Alcohol Analysis	
M2017-5213	1	99716	Alcohol Analysis	
M2017-5214	1	99719	Alcohol Analysis	
M2017-5215	1	99720	Alcohol Analysis	
M2017-5216	1	99755	Alcohol Analysis	
M2017-5217	1	99759	Alcohol Analysis	
M2017-5218	1	99762	Alcohol Analysis	

Worklist: 2036


<u>LAB CASE</u>	<u>ITEM</u>	<u>TASK_ID</u>	<u>DESCRIPTION</u>
M2017-5221	1	99903	Alcohol Analysis
M2017-5236	1	100005	Alcohol Analysis
M2017-5240	1	100010	Alcohol Analysis
P2017-2582	1	98731	Alcohol Analysis
P2017-2583	1	98732	Alcohol Analysis
P2017-2585	1	98734	Alcohol Analysis



JG

ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STD BLK 1
 Laboratory : Meridian
 Injection Date : Nov 17, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

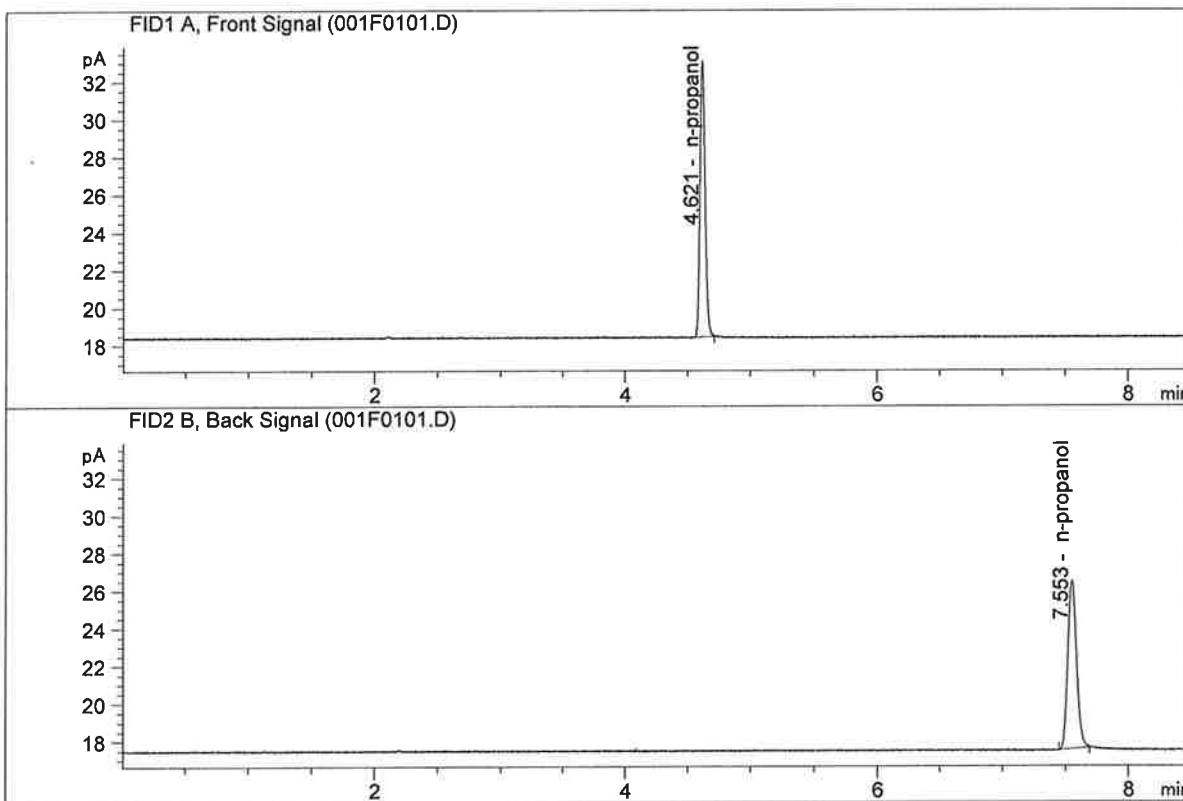


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	41.69909	1.0000	g/100cc
4.	n-Propanol	Column 2:	43.17113	1.0000	g/100cc

JK

ISP Forensic Services Blood Alcohol Report

Sample Name : MIX VOL FN09231404
 Laboratory : Meridian
 Injection Date : Nov 17, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

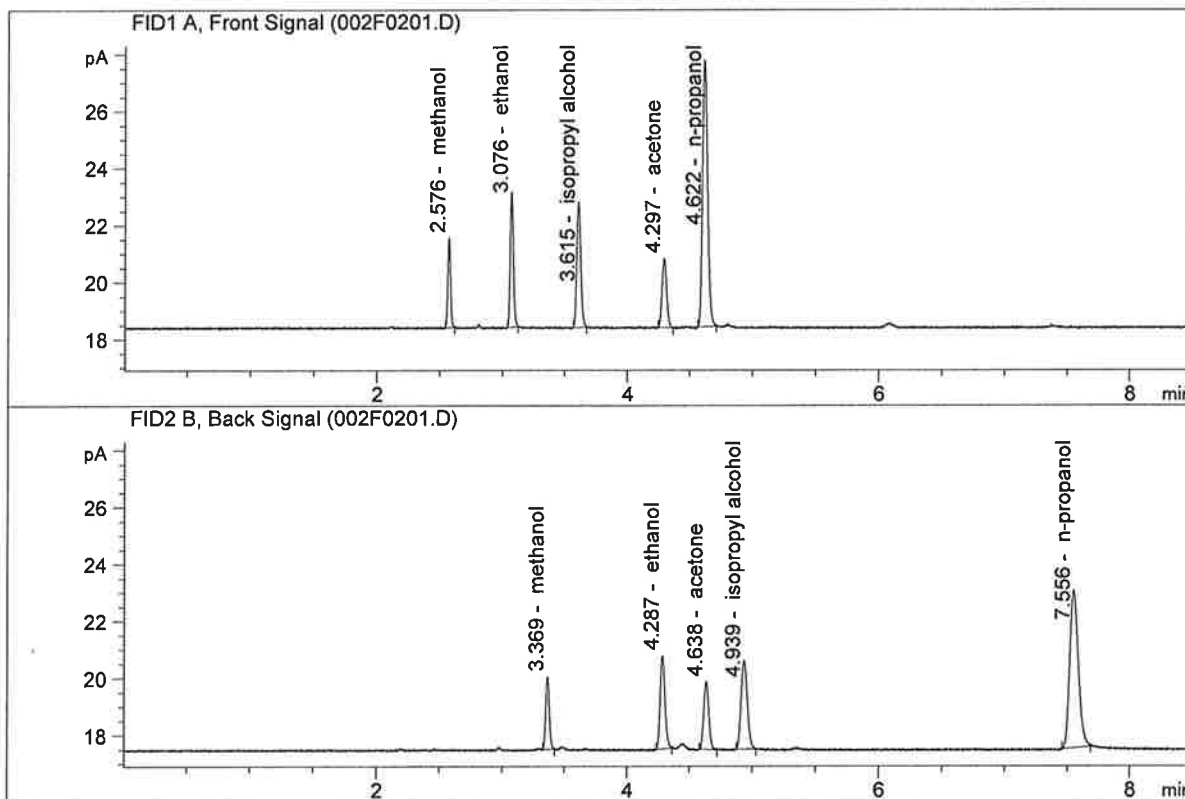

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	8.52608	0.1529	g/100cc
2.	Ethanol	Column 2:	8.74649	0.1533	g/100cc
3.	n-Propanol	Column 1:	26.50290	1.0000	g/100cc
4.	n-Propanol	Column 2:	26.58790	1.0000	g/100cc

Je

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC1-1

Analysis Date(s): 17 Nov 2017

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.0771	0.0779	0.0008	0.0775	0.0776	
(g/100cc)	0.0772	0.0785	0.0013	0.0778		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: ALCOHOL.M
Hamilton Auto-Dilutor Serial Number:
MD96BC1382/MD94AM10010

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.077	0.073	0.081	0.004

	Reported Result	
	0.077	

Calibration and control data are stored centrally.

Issued: 12/30/2016


Volatiles BAC Calculation Spreadsheet Rev 4

Issuing Authority: Quality Manager

JG

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-1-A
 Laboratory : Meridian
 Injection Date : Nov 17, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

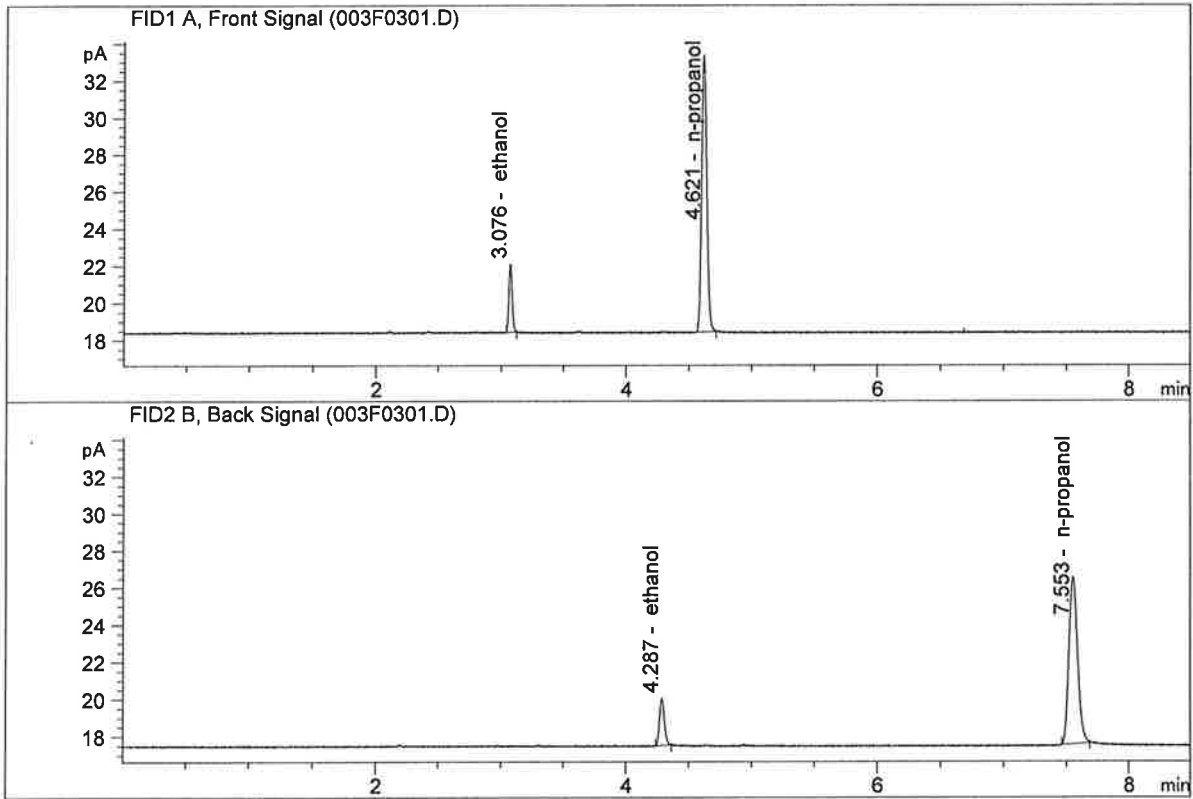


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	6.80884	0.0771	g/100cc
2.	Ethanol	Column 2:	6.86040	0.0779	g/100cc
3.	n-Propanol	Column 1:	42.48708	1.0000	g/100cc
4.	n-Propanol	Column 2:	43.09717	1.0000	g/100cc

JA

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-1-B
 Laboratory : Meridian
 Injection Date : Nov 17, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

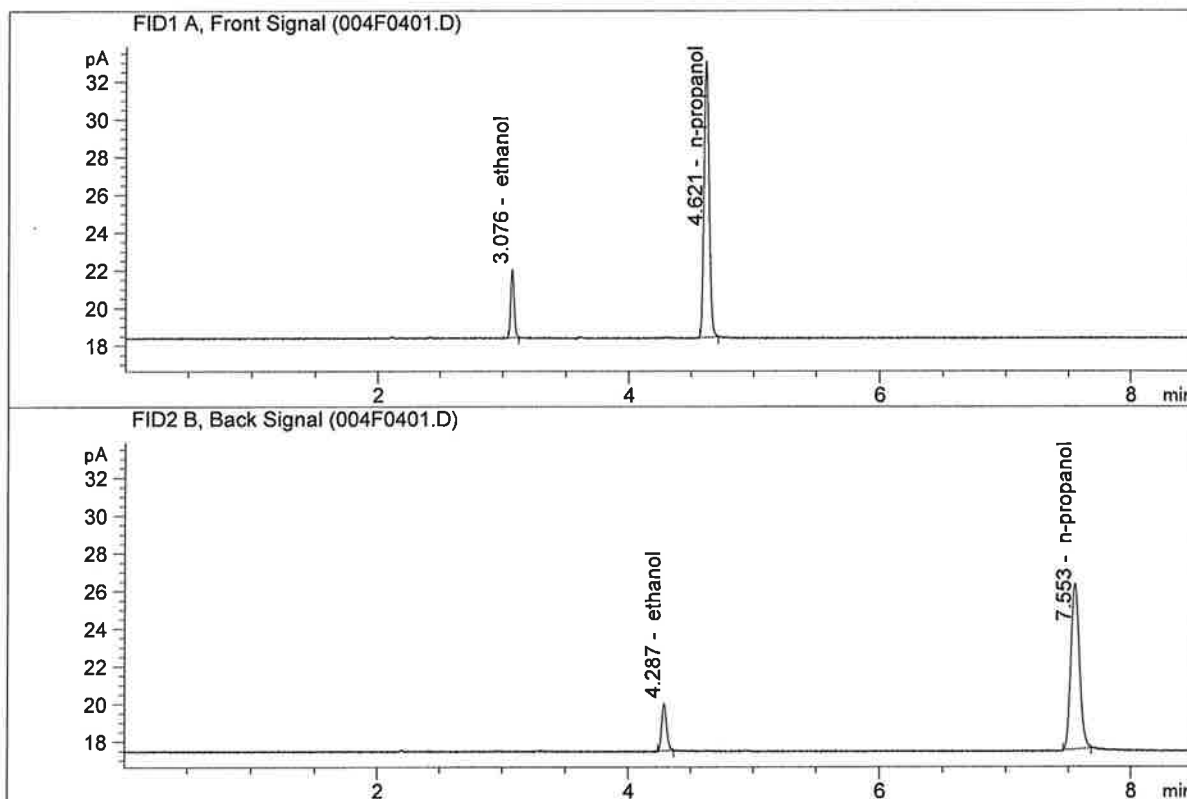

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	6.69402	0.0772	g/100cc
2.	Ethanol	Column 2:	6.78430	0.0785	g/100cc
3.	n-Propanol	Column 1:	41.73120	1.0000	g/100cc
4.	n-Propanol	Column 2:	42.23965	1.0000	g/100cc

JG

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: 0.08 FN10281510

Analysis Date(s): 17 Nov 2017

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.0802	0.0807	0.0005	0.0804	0.0808	
(g/100cc)	0.0806	0.0817	0.0011	0.0811		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: ALCOHOL.M
Hamilton Auto-Dilutor Serial Number:
MD96BC1382/MD94AM10010

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.080	0.076	0.084	0.004

	Reported Result	
	0.080	

Calibration and control data are stored centrally.

Issued: 12/30/2016


Volatiles BAC Calculation Spreadsheet Rev 4

Issuing Authority: Quality Manager

JG

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.08 FN10281510-A
 Laboratory : Meridian
 Injection Date : Nov 17, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

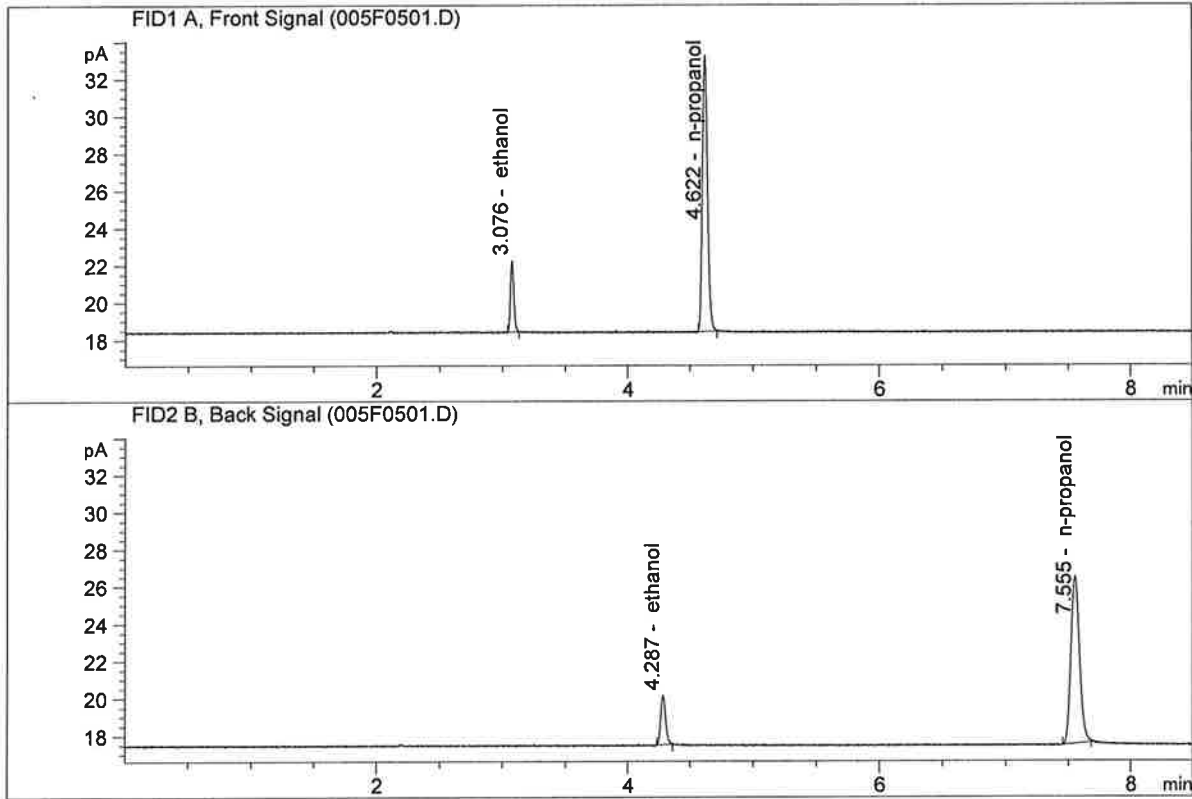


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.06452	0.0802	g/100cc
2.	Ethanol	Column 2:	7.10614	0.0807	g/100cc
3.	n-Propanol	Column 1:	42.35055	1.0000	g/100cc
4.	n-Propanol	Column 2:	42.92138	1.0000	g/100cc

UG

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.08 FN10281510-B
 Laboratory : Meridian
 Injection Date : Nov 17, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

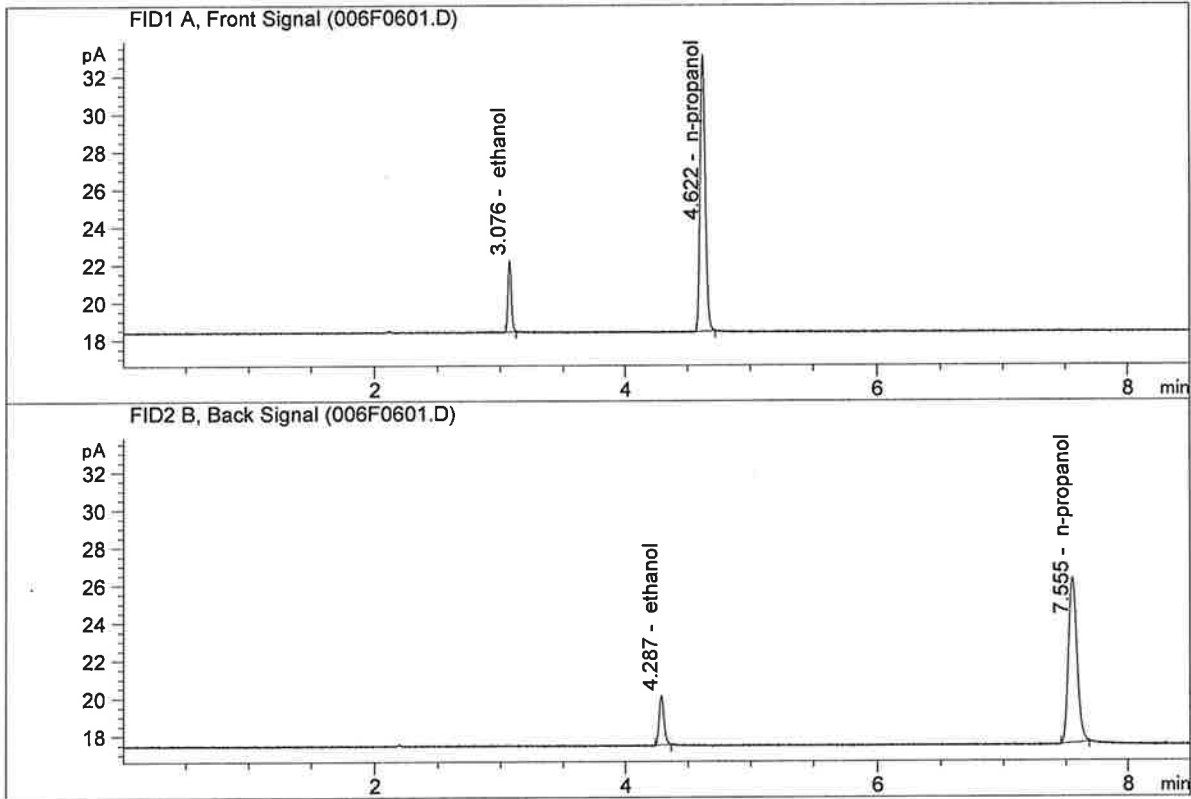

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.00279	0.0806	g/100cc
2.	Ethanol	Column 2:	7.07834	0.0817	g/100cc
3.	n-Propanol	Column 1:	41.75983	1.0000	g/100cc
4.	n-Propanol	Column 2:	42.18971	1.0000	g/100cc

JG

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC2-1

Analysis Date(s): 17 Nov 2017

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.2015	0.2000	0.0015	0.2007	0.1998	
(g/100cc)	0.1995	0.1983	0.0012	0.1989		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: ALCOHOL.M
Hamilton Auto-Dilutor Serial Number:
MD96BC1382/MD94AM10010

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.199	0.189	0.209	0.010

	Reported Result	
	0.199	

Calibration and control data are stored centrally.

Issued: 12/30/2016


Volatiles BAC Calculation Spreadsheet Rev 4

Issuing Authority: Quality Manager

JG

ISP Forensic Services Blood Alcohol Report

Sample Name : QC2-1-A
 Laboratory : Meridian
 Injection Date : Nov 17, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

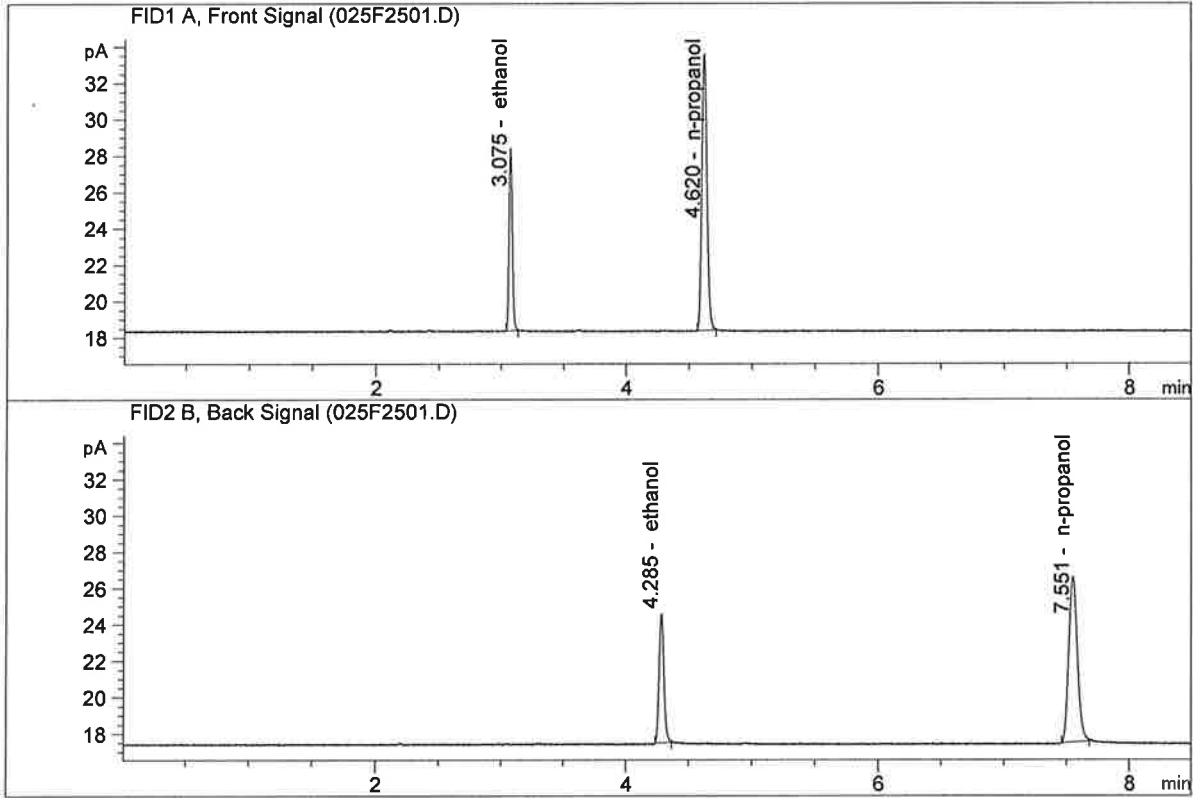


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	18.45054	0.2015	g/100cc
2.	Ethanol	Column 2:	18.87427	0.2000	g/100cc
3.	n-Propanol	Column 1:	43.38151	1.0000	g/100cc
4.	n-Propanol	Column 2:	43.47470	1.0000	g/100cc

JG

ISP Forensic Services Blood Alcohol Report

Sample Name : QC2-1-B
 Laboratory : Meridian
 Injection Date : Nov 17, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

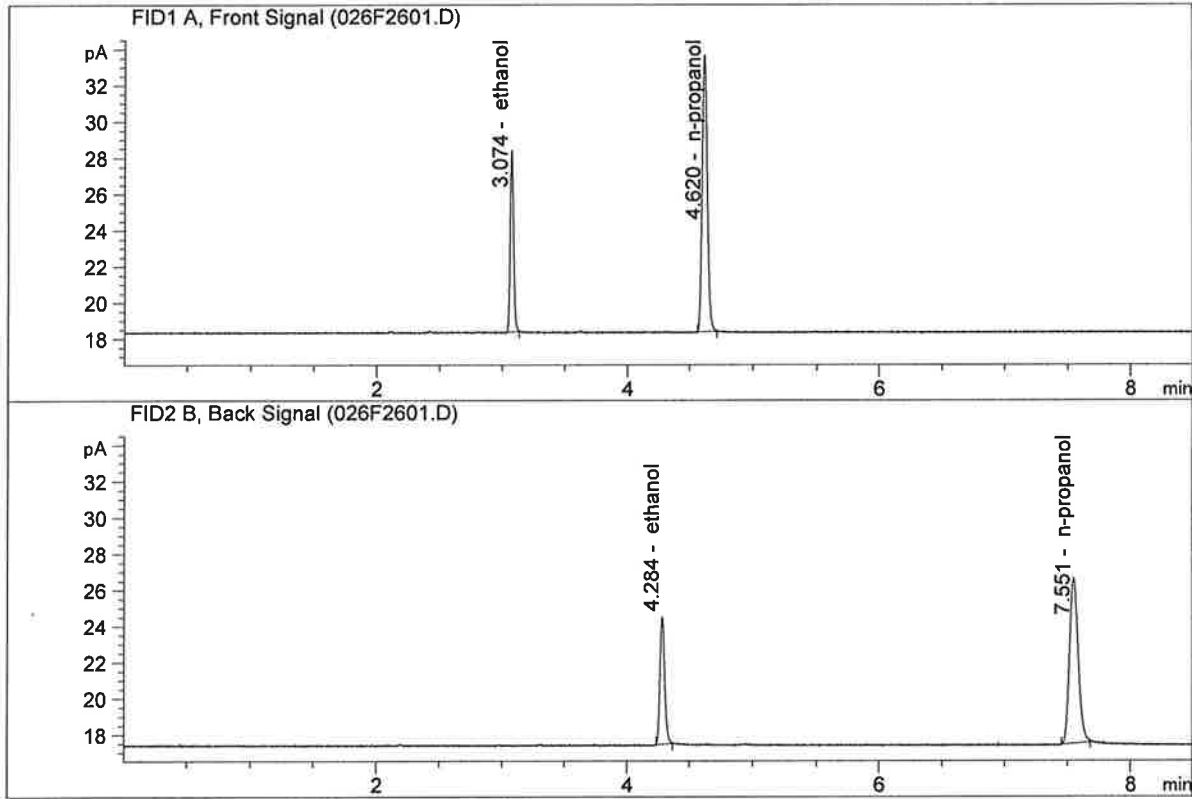

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	18.31377	0.1995	g/100cc
2.	Ethanol	Column 2:	18.79566	0.1983	g/100cc
3.	n-Propanol	Column 1:	43.51007	1.0000	g/100cc
4.	n-Propanol	Column 2:	43.67220	1.0000	g/100cc

56

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC1-2

Analysis Date(s): 18 Nov 2017

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.0820	0.0832	0.0012	0.0826	0.0825	
(g/100cc)	0.0819	0.0831	0.0012	0.0825		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: ALCOHOL.M
Hamilton Auto-Dilutor Serial Number:
MD96BC1382/MD94AM10010

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.082	0.077	0.087	0.005

	Reported Result	
	0.082	

Calibration and control data are stored centrally.

Issued: 12/30/2016


Volatiles BAC Calculation Spreadsheet Rev 4

Issuing Authority: Quality Manager



ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-2-A
 Laboratory : Meridian
 Injection Date : Nov 18, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

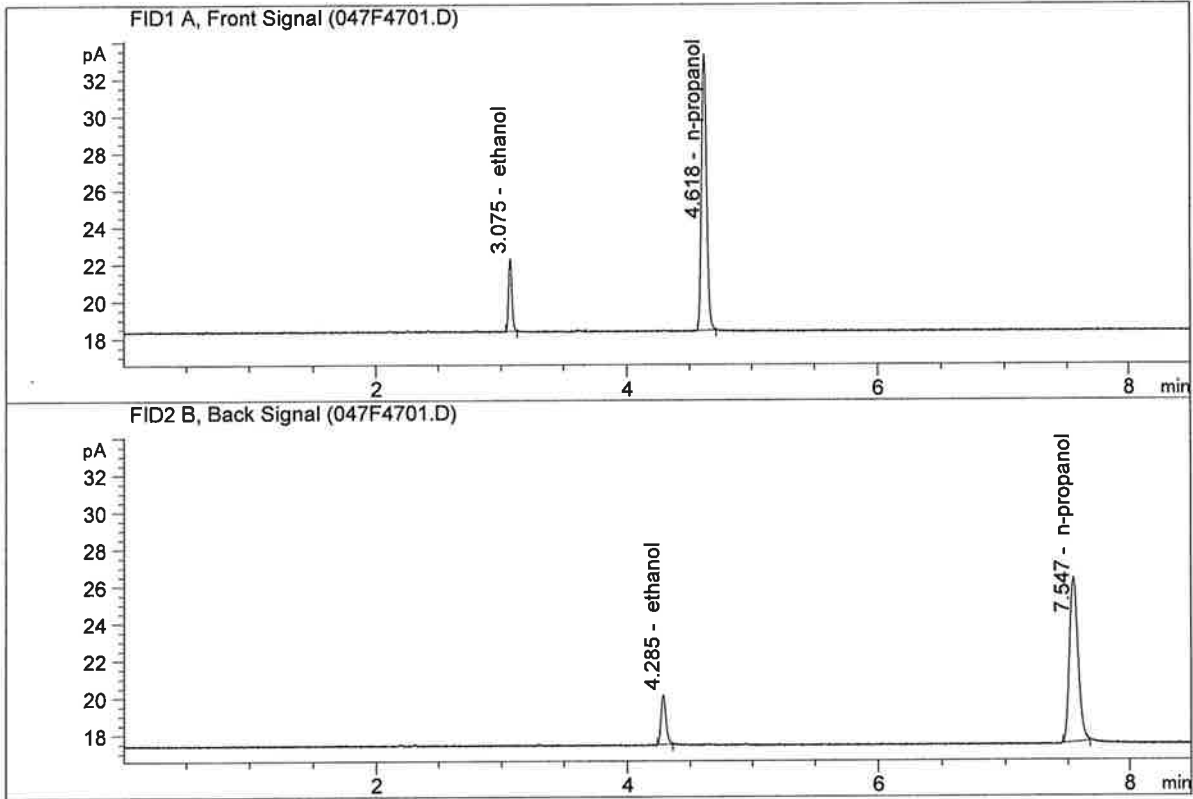


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.20554	0.0820	g/100cc
2.	Ethanol	Column 2:	7.21062	0.0832	g/100cc
3.	n-Propanol	Column 1:	42.19651	1.0000	g/100cc
4.	n-Propanol	Column 2:	42.09205	1.0000	g/100cc

ck

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-2-B
 Laboratory : Meridian
 Injection Date : Nov 18, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

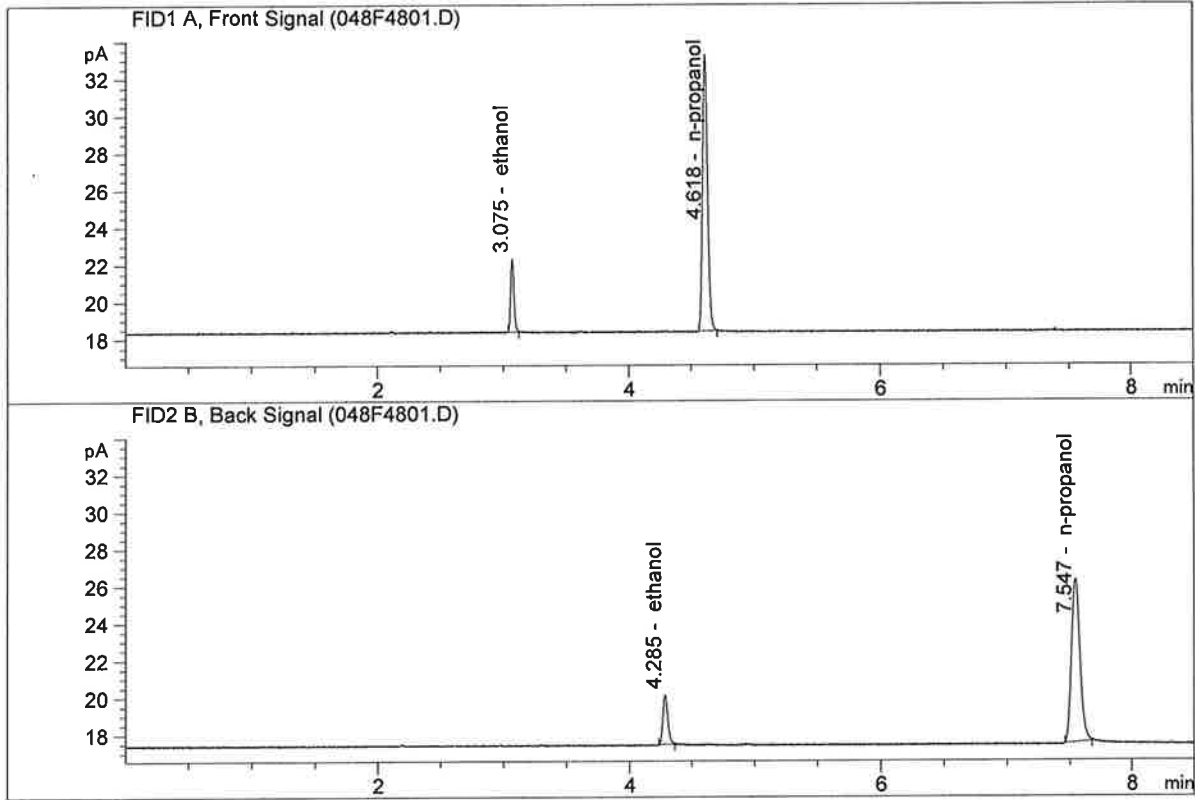

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.18450	0.0819	g/100cc
2.	Ethanol	Column 2:	7.18655	0.0831	g/100cc
3.	n-Propanol	Column 1:	42.11341	1.0000	g/100cc
4.	n-Propanol	Column 2:	42.01639	1.0000	g/100cc

JG

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC2-2

Analysis Date(s): 18 Nov 2017

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.2111	0.2107	0.0004	0.2109	0.2065	
(g/100cc)	0.2028	0.2017	0.0011	0.2022		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: ALCOHOL.M
Hamilton Auto-Dilutor Serial Number:
MD96BC1382/MD94AM10010

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.206	0.195	0.217	0.011

	Reported Result	
	0.206	

Calibration and control data are stored centrally.

Issued: 12/30/2016


Volatiles BAC Calculation Spreadsheet Rev 4

Issuing Authority: Quality Manager

JG

ISP Forensic Services Blood Alcohol Report

Sample Name : QC2-2-A
 Laboratory : Meridian
 Injection Date : Nov 18, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

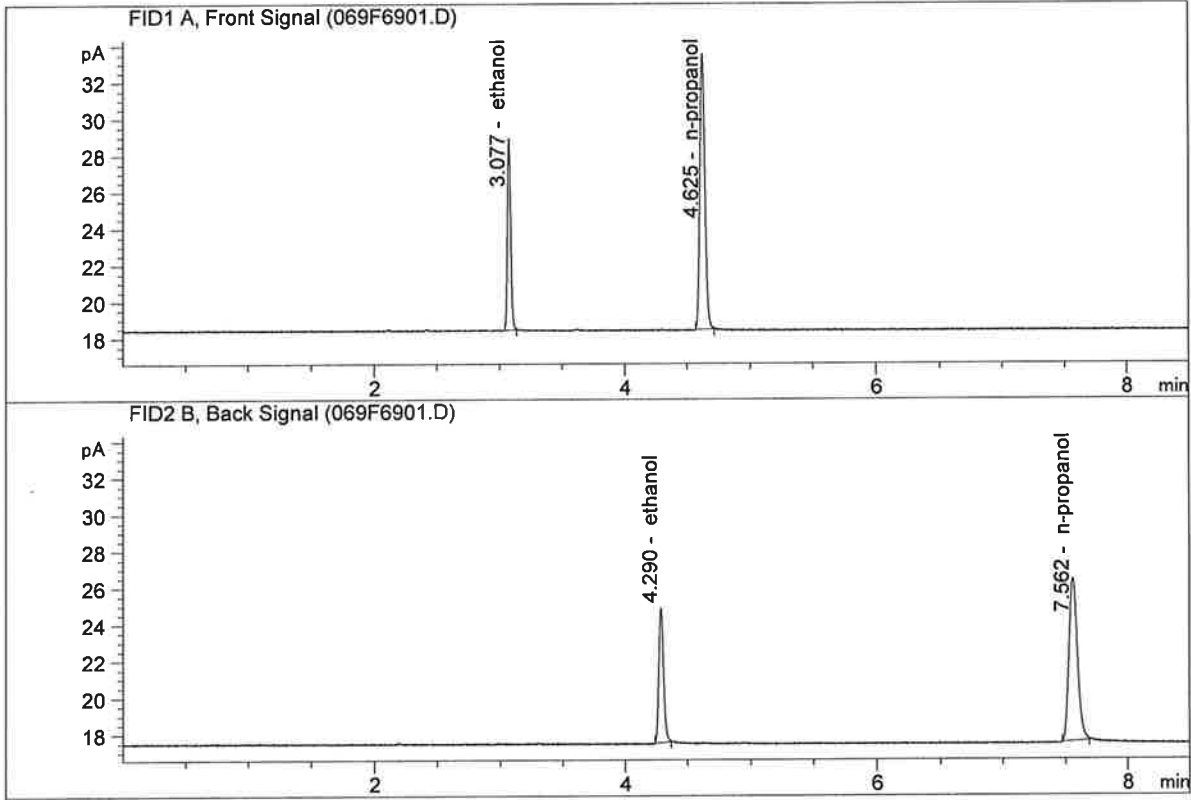


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	19.02834	0.2111	g/100cc
2.	Ethanol	Column 2:	19.50238	0.2107	g/100cc
3.	n-Propanol	Column 1:	42.69676	1.0000	g/100cc
4.	n-Propanol	Column 2:	42.55263	1.0000	g/100cc

JG

ISP Forensic Services Blood Alcohol Report

Sample Name : QC2-2-B
 Laboratory : Meridian
 Injection Date : Nov 18, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

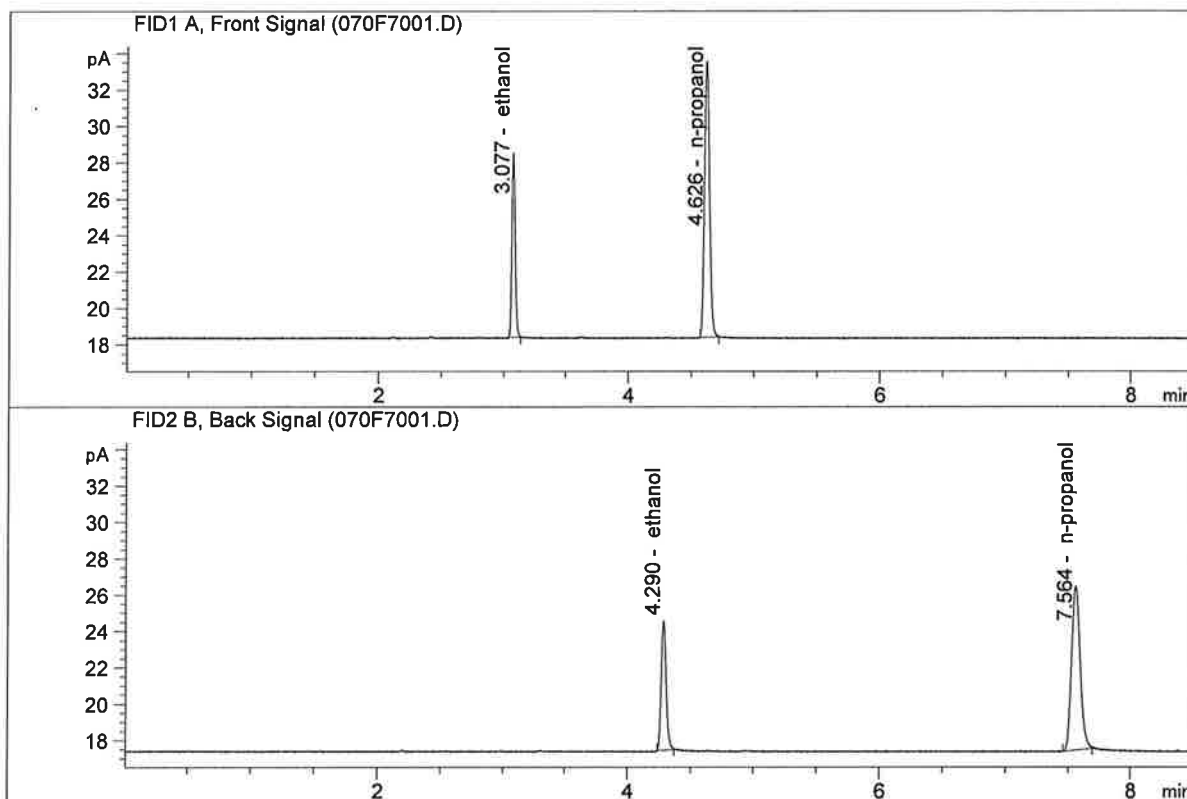


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	18.51835	0.2028	g/100cc
2.	Ethanol	Column 2:	18.97590	0.2017	g/100cc
3.	n-Propanol	Column 1:	43.25678	1.0000	g/100cc
4.	n-Propanol	Column 2:	43.32676	1.0000	g/100cc

JG

ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STD BLK
 Laboratory : Meridian
 Injection Date : Nov 18, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

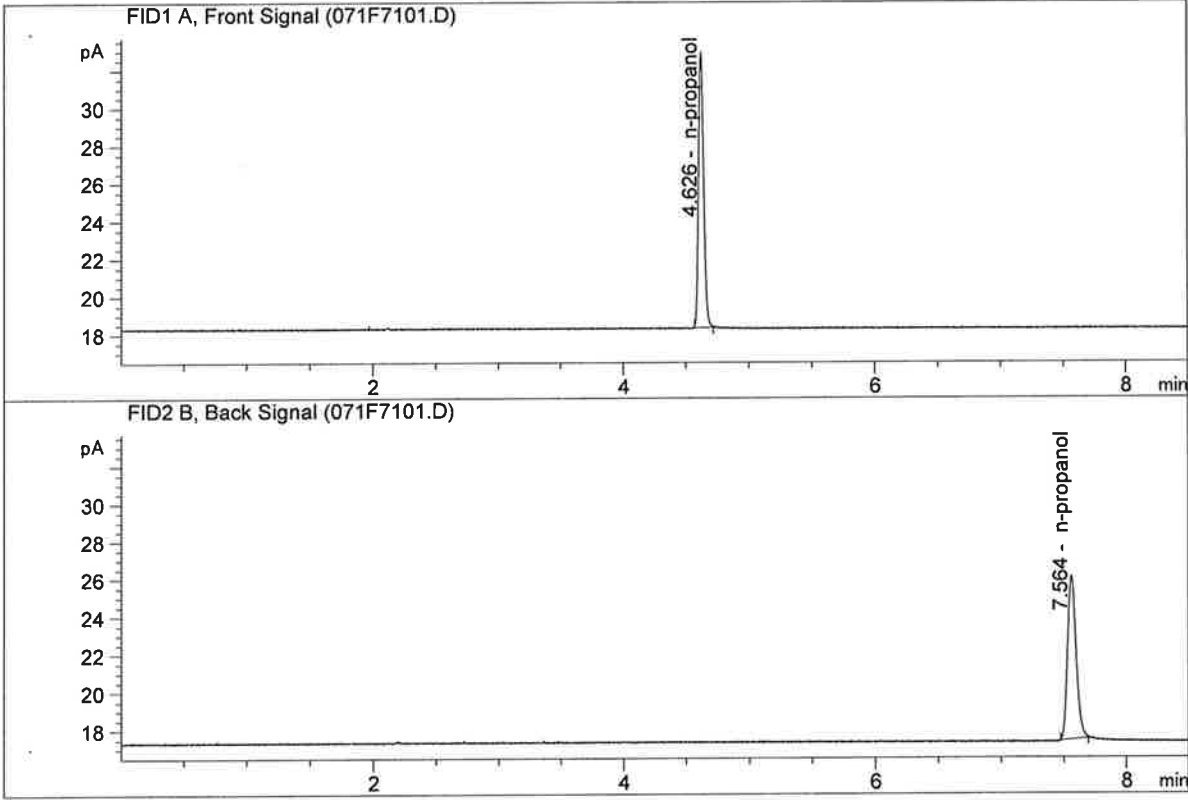


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	41.35999	1.0000	g/100cc
4.	n-Propanol	Column 2:	41.18482	1.0000	g/100cc

JG

ISP Forensic Services Blood Alcohol Report

Sample Name : DFE 111914OM
 Laboratory : Meridian
 Injection Date : Nov 18, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

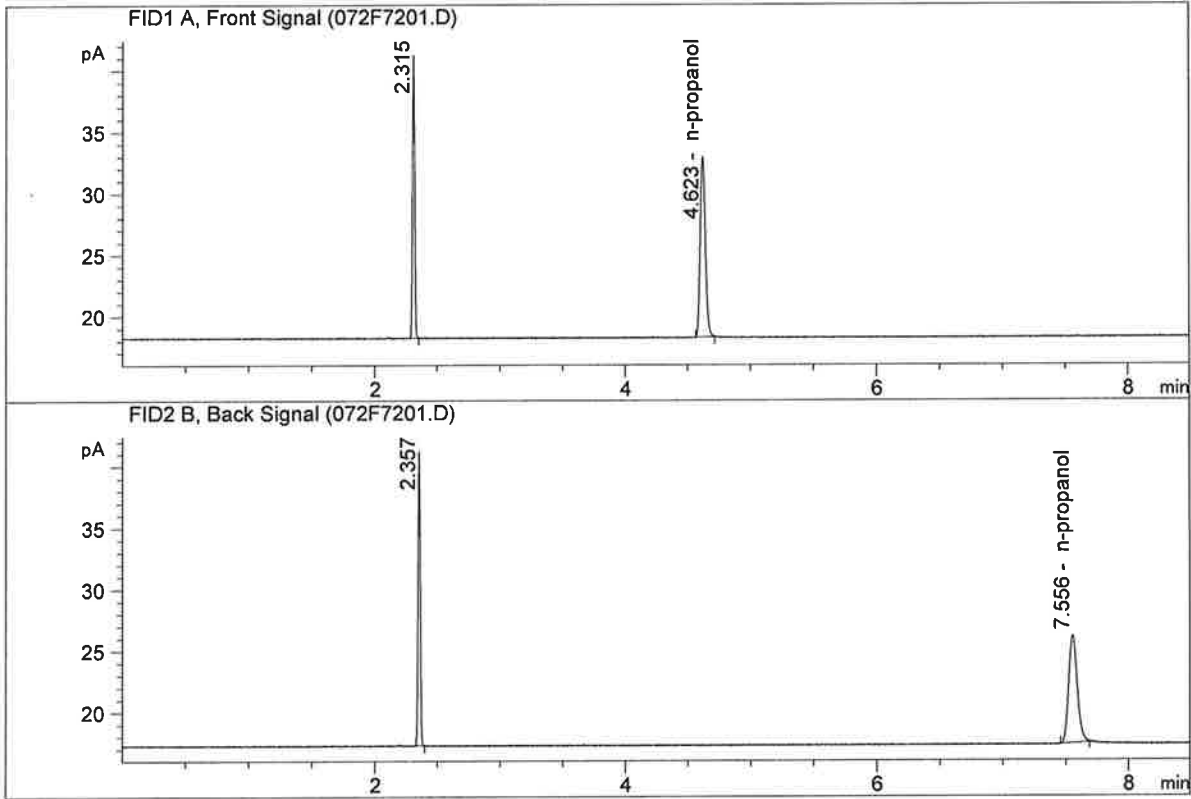


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	41.66875	1.0000	g/100cc
4.	n-Propanol	Column 2:	41.73472	1.0000	g/100cc

UG

ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STD BLK
 Laboratory : Meridian
 Injection Date : Nov 18, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

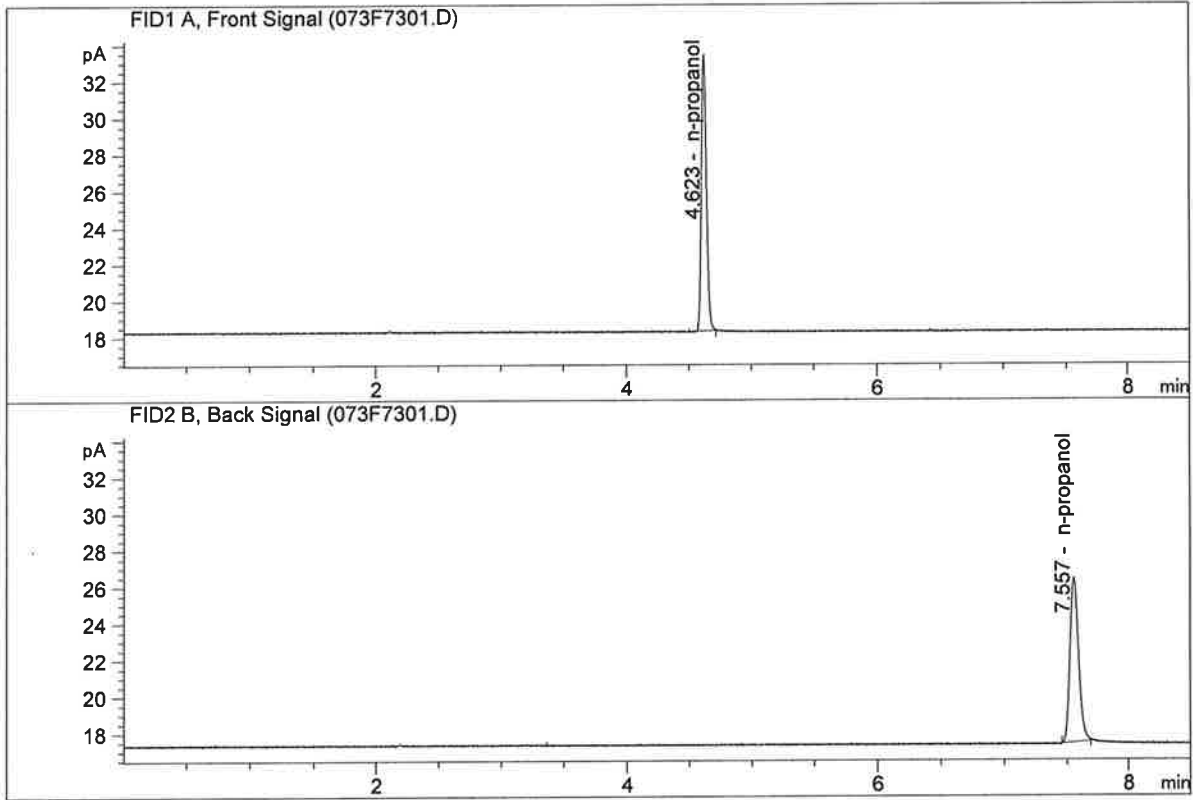


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	42.73918	1.0000	g/100cc
4.	n-Propanol	Column 2:	42.91892	1.0000	g/100cc

JA

ISP Forensic Services Blood Alcohol Report


Sample Name : TFE 111914
 Laboratory : Meridian
 Injection Date : Nov 18, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

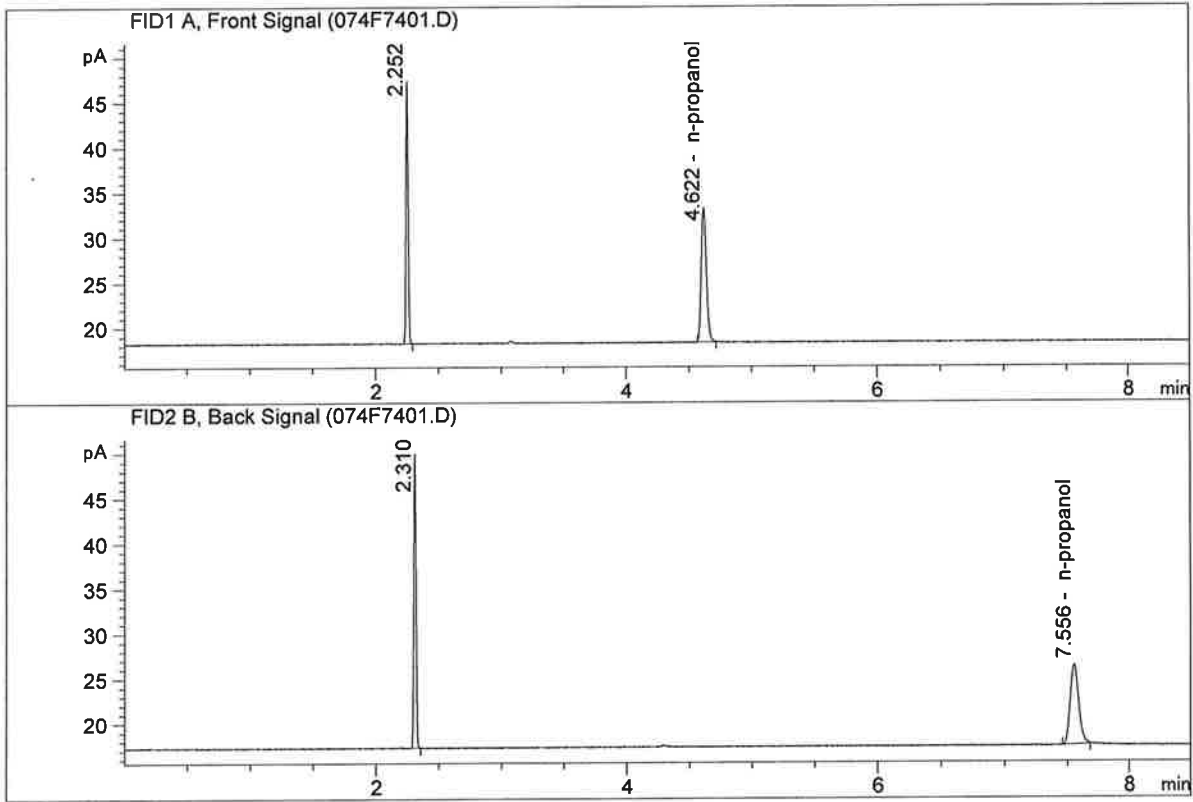

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	42.32698	1.0000	g/100cc
4.	n-Propanol	Column 2:	42.42755	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STD BLK
 Laboratory : Meridian
 Injection Date : Nov 18, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

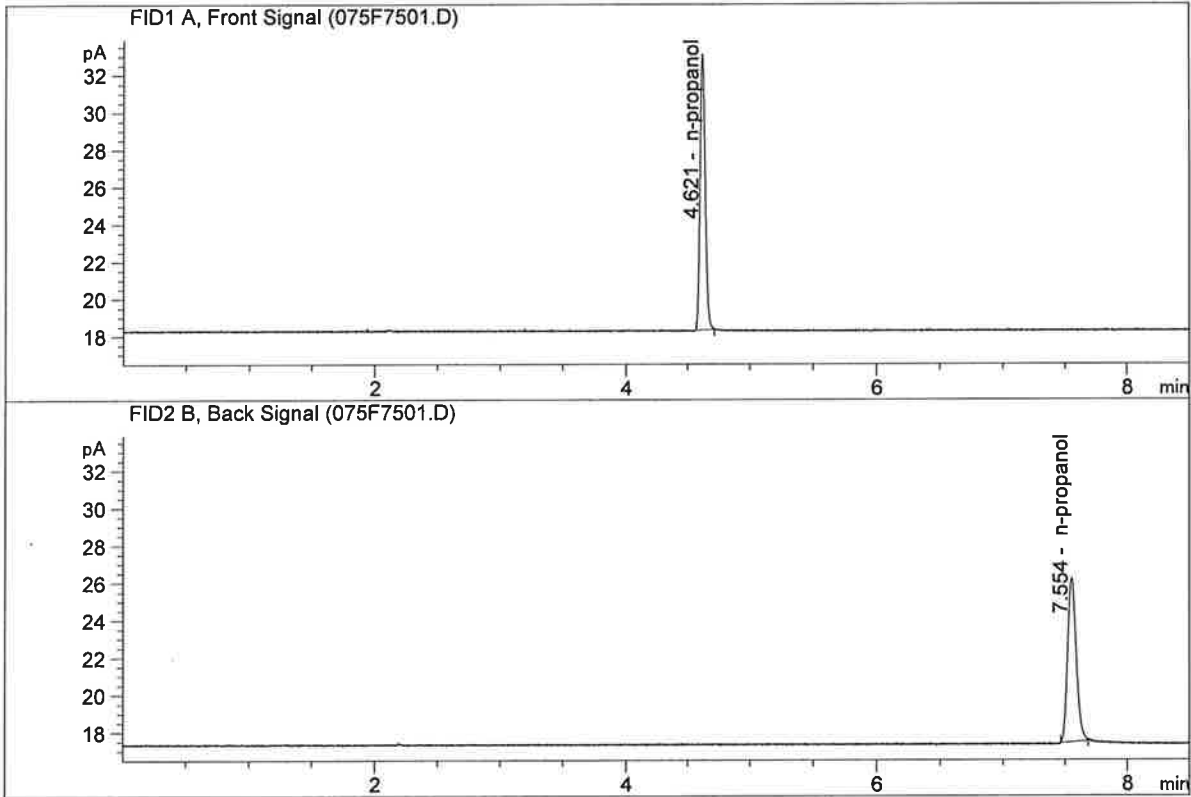

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	41.90515	1.0000	g/100cc
4.	n-Propanol	Column 2:	41.87521	1.0000	g/100cc

26

S a m p l e S u m m a r y

Sequence table: C:\Chem32\1\Data\11-17-17_SAMPLES\11-17-17_SAMPLES 2017-11-17 16-39-13\11-17-17_SAMPLES.S
 Data directory path: C:\Chem32\1\Data\11-17-17_SAMPLES\11-17-17_SAMPLES 2017-11-17 16-39-13\
 Logbook: C:\Chem32\1\Data\11-17-17_SAMPLES\11-17-17_SAMPLES 2017-11-17 16-39-13\11-17-17_SAMPLES.LOG
 Sequence start: 11/17/2017 4:54:05 PM
 Sequence Operator: SYSTEM
 Operator: SYSTEM
 Method file name: C:\Chem32\1\Data\11-17-17_SAMPLES\11-17-17_SAMPLES 2017-11-17 16-39-13\
 \ALCOHOL.M

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #	# Cmp
1	1	1	INTERNAL STD BLK	-	1.0000	001F0101.D		2
2	2	1	MIX VOL FN092314	-	1.0000	002F0201.D		10
3	3	1	QC1-1-A	-	1.0000	003F0301.D		4
4	4	1	QC1-1-B	-	1.0000	004F0401.D		4
5	5	1	0.08 FN10281510-	-	1.0000	005F0501.D		4
6	6	1	0.08 FN10281510-	-	1.0000	006F0601.D		4
7	7	1	M2017-5087-1-A	-	1.0000	007F0701.D		6
8	8	1	M2017-5087-1-B	-	1.0000	008F0801.D		6
9	9	1	M2017-5088-1-A	-	1.0000	009F0901.D		6
10	10	1	M2017-5088-1-B	-	1.0000	010F1001.D		6
11	11	1	M2017-5089-2-A	-	1.0000	011F1101.D		6
12	12	1	M2017-5089-2-B	-	1.0000	012F1201.D		6
13	13	1	M2017-5090-1-A	-	1.0000	013F1301.D		6
14	14	1	M2017-5090-1-B	-	1.0000	014F1401.D		6
15	15	1	M2017-5145-1-A	-	1.0000	015F1501.D		6
16	16	1	M2017-5145-1-B	-	1.0000	016F1601.D		6
17	17	1	M2017-5154-1-A	-	1.0000	017F1701.D		6
18	18	1	M2017-5154-1-B	-	1.0000	018F1801.D		6
19	19	1	M2017-5155-1-A	-	1.0000	019F1901.D		6
20	20	1	M2017-5155-1-B	-	1.0000	020F2001.D		6
21	21	1	P2017-2582-1-A	-	1.0000	021F2101.D		6
22	22	1	P2017-2582-1-B	-	1.0000	022F2201.D		6
23	23	1	P2017-2583-1-A	-	1.0000	023F2301.D		6
24	24	1	P2017-2583-1-B	-	1.0000	024F2401.D		6
25	25	1	QC2-1-A	-	1.0000	025F2501.D		4
26	26	1	QC2-1-B	-	1.0000	026F2601.D		4
27	27	1	P2017-2585-1-A	-	1.0000	027F2701.D		2
28	28	1	P2017-2585-1-B	-	1.0000	028F2801.D		2
29	29	1	M2017-5158-1-A	-	1.0000	029F2901.D		6
30	30	1	M2017-5158-1-B	-	1.0000	030F3001.D		6
31	31	1	M2017-5159-1-A	-	1.0000	031F3101.D		4
32	32	1	M2017-5159-1-B	-	1.0000	032F3201.D		4
33	33	1	M2017-5160-1-A	-	1.0000	033F3301.D		6
34	34	1	M2017-5160-1-B	-	1.0000	034F3401.D		5
35	35	1	M2017-5180-1-A	-	1.0000	035F3501.D		2
36	36	1	M2017-5180-1-B	-	1.0000	036F3601.D		2
37	37	1	M2017-5190-1-A	-	1.0000	037F3701.D		6
38	38	1	M2017-5190-1-B	-	1.0000	038F3801.D		6
39	39	1	M2017-5194-1-A	-	1.0000	039F3901.D		6
40	40	1	M2017-5194-1-B	-	1.0000	040F4001.D		6
41	41	1	M2017-5196-2-A	-	1.0000	041F4101.D		2
42	42	1	M2017-5196-2-B	-	1.0000	042F4201.D		2
43	43	1	M2017-5203-1-A	-	1.0000	043F4301.D		2

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #
44	44	1	M2017-5203-1-B	-	1.0000	044F4401.D	2
45	45	1	M2017-5204-1-A	-	1.0000	045F4501.D	4
46	46	1	M2017-5204-1-B	-	1.0000	046F4601.D	4
47	47	1	QC1-2-A	-	1.0000	047F4701.D	4
48	48	1	QC1-2-B	-	1.0000	048F4801.D	4
49	49	1	M2017-5205-1-A	-	1.0000	049F4901.D	4
50	50	1	M2017-5205-1-B	-	1.0000	050F5001.D	4
51	51	1	M2017-5213-1-A	-	1.0000	051F5101.D	6
52	52	1	M2017-5213-1-B	-	1.0000	052F5201.D	6
53	53	1	M2017-5214-1-A	-	1.0000	053F5301.D	6
54	54	1	M2017-5214-1-B	-	1.0000	054F5401.D	6
55	55	1	M2017-5215-1-A	-	1.0000	055F5501.D	5
56	56	1	M2017-5215-1-B	-	1.0000	056F5601.D	4
57	57	1	M2017-5216-1-A	-	1.0000	057F5701.D	6
58	58	1	M2017-5216-1-B	-	1.0000	058F5801.D	6
59	59	1	M2017-5217-1-A	-	1.0000	059F5901.D	6
60	60	1	M2017-5217-1-B	-	1.0000	060F6001.D	6
61	61	1	M2017-5218-1-A	-	1.0000	061F6101.D	6
62	62	1	M2017-5218-1-B	-	1.0000	062F6201.D	6
63	63	1	M2017-5221-1-A	-	1.0000	063F6301.D	6
64	64	1	M2017-5221-1-B	-	1.0000	064F6401.D	6
65	65	1	M2017-5236-1-A	-	1.0000	065F6501.D	6
66	66	1	M2017-5236-1-B	-	1.0000	066F6601.D	6
67	67	1	M2017-5240-1-A	-	1.0000	067F6701.D	4
68	68	1	M2017-5240-1-B	-	1.0000	068F6801.D	4
69	69	1	QC2-2-A	-	1.0000	069F6901.D	4
70	70	1	QC2-2-B	-	1.0000	070F7001.D	4
71	71	1	INTERNAL STD BLK	-	1.0000	071F7101.D	2
72	72	1	DFE 111914OM	-	1.0000	072F7201.D	2
73	73	1	INTERNAL STD BLK	-	1.0000	073F7301.D	2
74	74	1	TFE 111914	-	1.0000	074F7401.D	2
75	75	1	INTERNAL STD BLK	-	1.0000	075F7501.D	2

Method file name: C:\Chem32\1\Data\11-17-17_SAMPLES\11-17-17_SAMPLES 2017-11-17 16-39-13
 \SHUTDOWN.M

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #
76	76	1	EMPTY	-	1.0000	076F7601.D	0

JK