


Worklist: 3869

<u>LAB_CASE</u>	<u>ITEM</u>	<u>ITEM_TYPE</u>	<u>DESCRIPTION</u>
M2019-5366	1	BCK	Alcohol Analysis
M2019-5367	1	BCK	Alcohol Analysis
M2019-5368	1	BCK	Alcohol Analysis
M2019-5369	1	BCK	Alcohol Analysis
M2019-5404	1	BCK	Alcohol Analysis
P2019-3548	1	BCK	Alcohol Analysis
P2019-3565	1	BCK	Alcohol Analysis
P2019-3566	1	BCK	Alcohol Analysis
P2019-3567	1	BCK	Alcohol Analysis
P2019-3572	1	BCK	Alcohol Analysis
P2019-3584	1	BCK	Alcohol Analysis
P2019-3588	1	BCK	Alcohol Analysis
P2019-3602	1	BCK	Alcohol Analysis
P2019-3603	1	BCK	Alcohol Analysis
P2019-3605	1	BCK	Alcohol Analysis
P2019-3614	1	BCK	Alcohol Analysis
P2019-3615	1	BCK	Alcohol Analysis

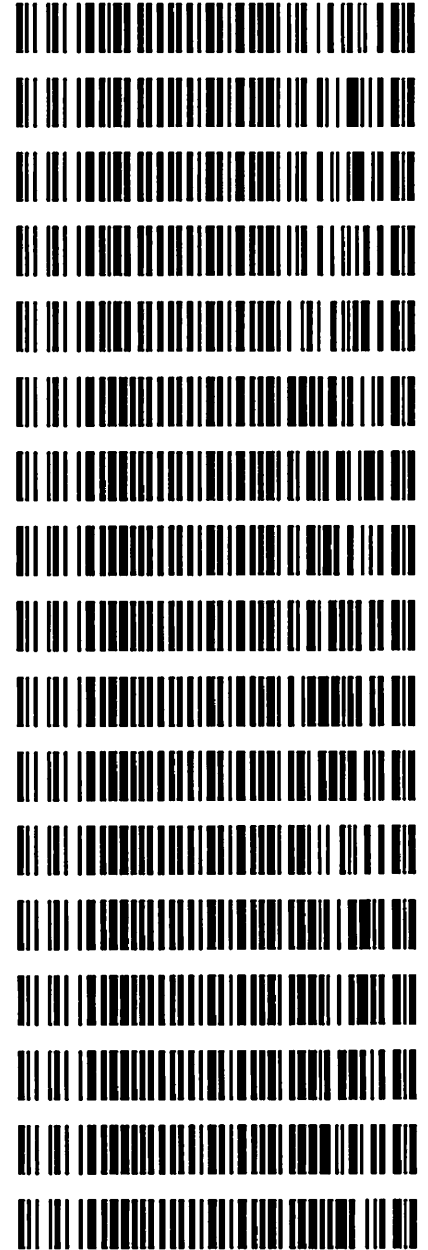

Quantitative Analysis for Ethanol & Qualitative Analysis for Other Volatiles

Analytical Method(s): 1.0

Device: Hamilton MICROLAB 600A Liquid Processor/Dilutor Serial Number: ML600HC11378

Volatiles Quality Assurance Controls

Run Date(s): 12/5/19

Calibration Date: 11/29/19

Control level	Expiration	Lot #	Target Value	Acceptable Range	Overall Results
Level 1	Jan-22	1801036	0.0812	0.0731-0.0893	0.0810 g/100cc 0.0810 g/100cc g/100cc
Level 2	Mar-22	1803028	0.2035	0.1832-0.2238	0.1959 g/100cc g/100cc
Multi-Component mixture:			Lot #	FN06041502	OK
Curve Fit:		Column 1	0.99999	Column 2	0.99995

Ethanol Calibration Reference Material

Calibrator level	Target Value	Acceptable Range	Column 1	Column 2	Precision	Mean
50	0.050	0.045 - 0.055	0.5040	0.0523	0.4517	0.2781
100	0.100	0.090 - 0.110	0.0998	0.0995	0.0003	0.0996
200	0.200	0.180 - 0.220	0.1992	0.1975	0.0017	0.1983
300	0.300	0.270 - 0.330	0.3007	0.2996	0.0011	0.3001
500	0.500	0.450 - 0.550	0.4999	0.5011	0.0012	0.5005

Aqueous Controls

Control level	Target Value	Acceptable Range	Overall Results
80	0.080	0.076 - 0.084	0.081 g/100cc

W

=====
Calibration Table
=====

General Calibration Setting

Calib. Data Modified : Friday, November 29, 2019 9:46:46 AM
Signals calculated separately : No

Rel. Reference Window : 0.000 %
Abs. Reference Window : 0.100 min
Rel. Non-ref. Window : 0.000 %
Abs. Non-ref. Window : 0.100 min
Uncalibrated Peaks : not reported
Partial Calibration : Yes, identified peaks are recalibrated
Correct All Ret. Times: No, only for identified peaks

Curve Type : Linear
Origin : Ignored
Weight : Equal

Recalibration Settings:
Average Response : Average all calibrations
Average Retention Time: Floating Average New 75%

Calibration Report Options :
Printout of recalibrations within a sequence:
Calibration Table after Recalibration
Normal Report after Recalibration
If the sequence is done with bracketing:
Results of first cycle (ending previous bracket)

Default Sample ISTD Information (if not set in sample table):

ISTD #	ISTD Amount [g/100cc]	Name
1	1.00000	n-propanol
2	1.00000	n-propanol

Signal Details

Signal 1: FID1 A, Front Signal
Signal 2: FID2 B, Back Signal

Overview Table

RT	Sig	Lvl	Amount [g/100cc]	Area	Rsp.Factor	Ref	ISTD #	Compound
2.586	1	1	1.00000	3.69669	2.70512e-1	No	No	1 methanol
2.809	1	1	1.00000	4.26100	2.34687e-1	No	No	2 Acetaldehyde
2.977	2	1	1.00000	4.26100	2.34687e-1	No	No	2 Acetaldehyde
3.075	1	1	5.00000e-2	4.32853	1.15513e-2	No	No	1 ethanol
		2	1.00000e-1	8.81372	1.13460e-2			
		3	2.00000e-1	17.73868	1.12748e-2			
		4	3.00000e-1	26.62050	1.12695e-2			
		5	5.00000e-1	44.55405	1.12223e-2			
3.388	2	1	1.00000	4.26062	2.34707e-1	No	No	2 methanol
3.628	1	1	1.00000	9.73055	1.02769e-1	No	No	1 isopropyl alcohol
4.285	2	1	5.00000e-2	4.45698	1.12184e-2	No	No	2 ethanol
		2	1.00000e-1	9.04277	1.10586e-2			
		3	2.00000e-1	18.43505	1.08489e-2			
		4	3.00000e-1	27.88322	1.07592e-2			
		5	5.00000e-1	47.09054	1.06178e-2			
4.308	1	1	1.00000	6.49940	1.53860e-1	No	No	1 acetone
4.620	1	1	1.00000	45.35659	2.20475e-2	No	Yes	1 n-propanol
		2	1.00000	46.09383	2.16949e-2			
		3	1.00000	46.20026	2.16449e-2			
		4	1.00000	45.82462	2.18223e-2			
		5	1.00000	46.05164	2.17148e-2			
4.661	2	1	1.00000	6.89301	1.45075e-1	No	No	2 acetone
4.969	2	1	1.00000	10.70642	9.34019e-2	No	No	2 isopropyl alcohol
7.550	2	1	1.00000	47.21875	2.11780e-2	No	Yes	2 n-propanol
		2	1.00000	47.70168	2.09636e-2			
		3	1.00000	47.67413	2.09757e-2			
		4	1.00000	47.07686	2.12419e-2			
		5	1.00000	47.19093	2.11905e-2			


Peak Sum Table

No Entries in table


51 Warnings or Errors (10 first messages follow) :

- Warning : Curve requires more calibration points., (methanol)
- Warning : Curve requires more calibration points. at 2.586 min, signal 1
- Warning : Curve requires more calibration points. at 2.809 min, signal 1
- Warning : Curve requires more calibration points. at 2.977 min, signal 2
- Warning : Curve requires more calibration points. at 3.388 min, signal 2
- Warning : Curve requires more calibration points. at 3.628 min, signal 1
- Warning : Curve requires more calibration points. at 4.308 min, signal 1
- Warning : Curve requires more calibration points. at 4.62 min, signal 1
- Warning : Curve requires more calibration points. at 4.661 min, signal 2
- Warning : Curve requires more calibration points. at 4.969 min, signal 2


=====
 Calibration Curves
 =====

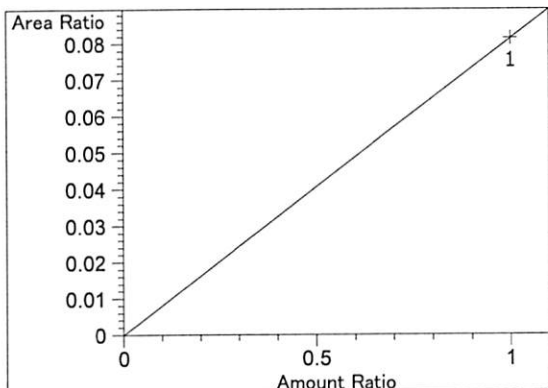


methanol at exp. RT: 2.586
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 8.15029e-2
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio

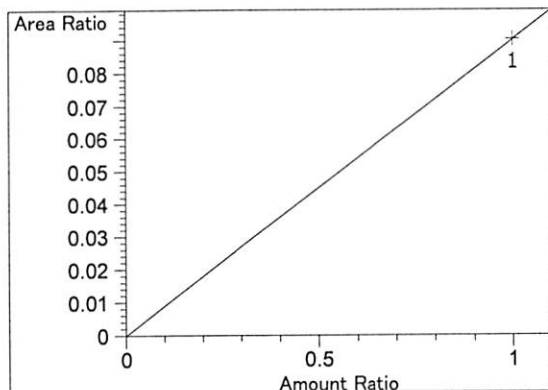

Acetaldehyde at exp. RT: 2.809
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 9.02396e-2
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio

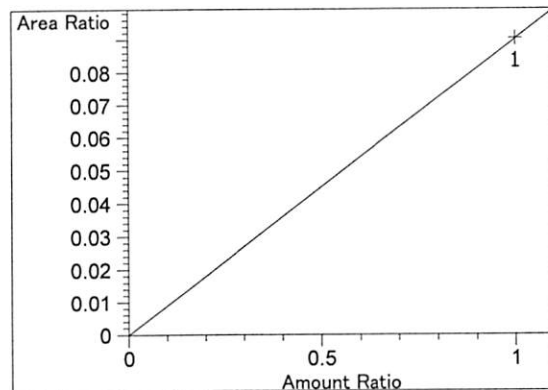


Acetaldehyde at exp. RT: 2.977
 FID2 B, Back Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 9.02396e-2
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio

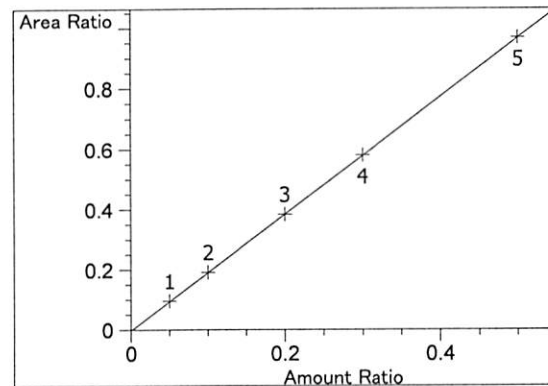


ethanol at exp. RT: 3.075
 FID1 A, Front Signal
 Correlation: 0.99999
 Residual Std. Dev.: 0.00133
 Formula: $y = mx + b$
 m: 1.94008
 b: -2.41805e-3
 x: Amount Ratio
 y: Area Ratio


W

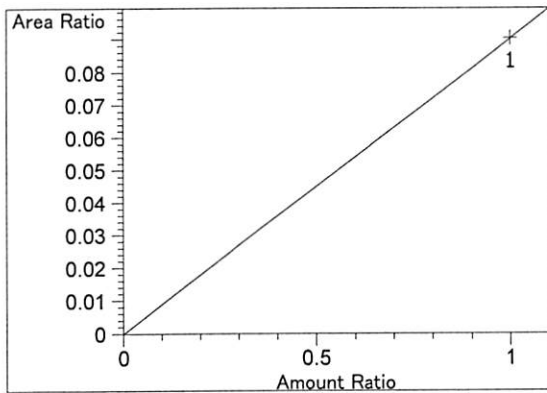


methanol at exp. RT: 3.388
 FID2 B, Back Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: $9.02316e-2$
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio

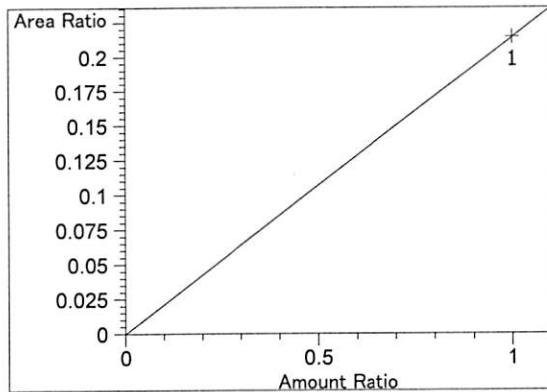

isopropyl alcohol at exp. RT: 3.628
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: $2.14535e-1$
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio

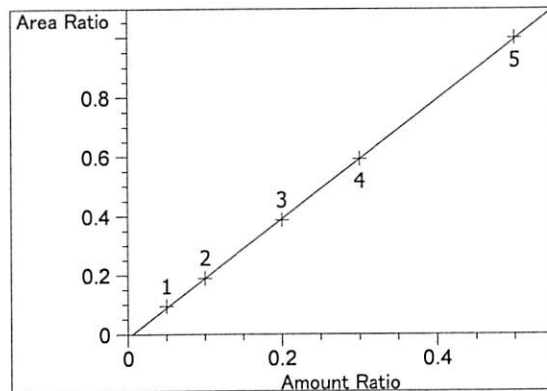


ethanol at exp. RT: 4.285
 FID2 B, Back Signal
 Correlation: 0.99995
 Residual Std. Dev.: 0.00420
 Formula: $y = mx + b$
 m: 2.01290
 b: $-1.08045e-2$
 x: Amount Ratio
 y: Area Ratio

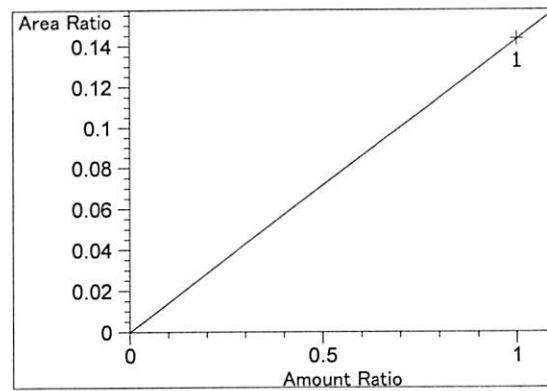


acetone at exp. RT: 4.308
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: $1.43296e-1$
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio


Handwritten signature

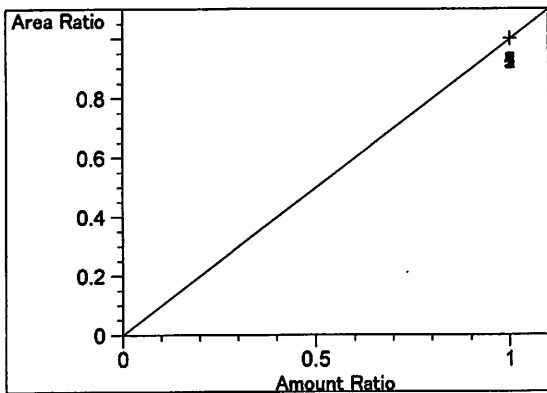


n-propanol at exp. RT: 4.620
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 1.00000
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio

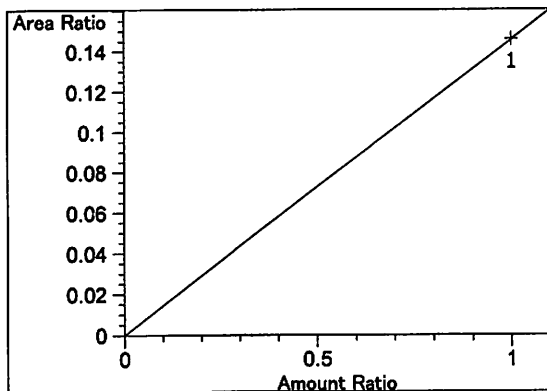

acetone at exp. RT: 4.661
 FID2 B, Back Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 1.45980e-1
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio

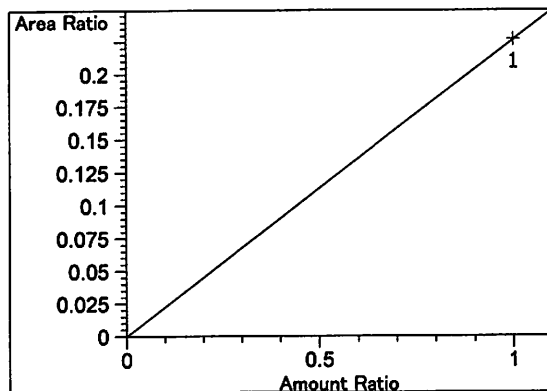

isopropyl alcohol at exp. RT: 4.969
 FID2 B, Back Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 2.26741e-1
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio

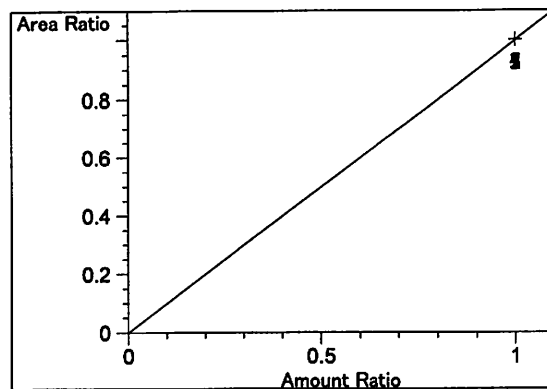


n-propanol at exp. RT: 7.550
 FID2 B, Back Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 1.00000
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio

=====

W

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.050 FN05211804
 Laboratory : Meridian
 Injection Date : Nov 29, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

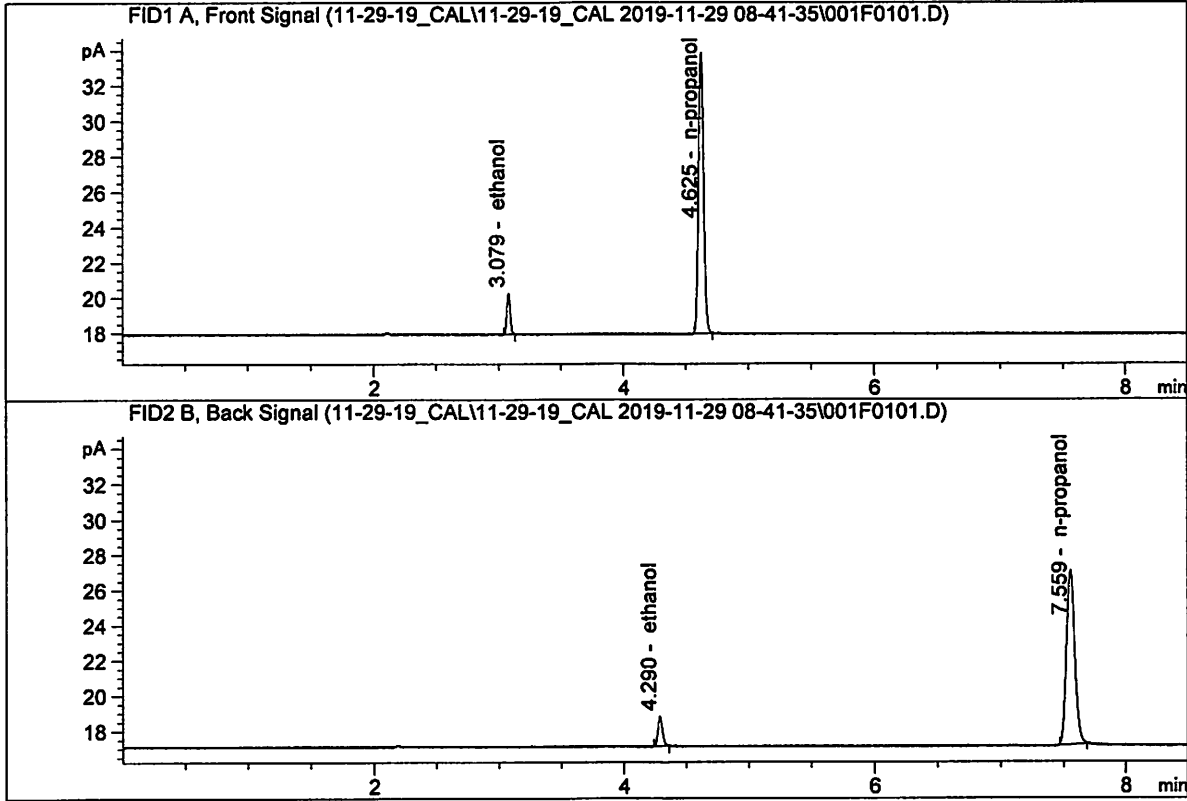


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	4.32853	0.0504	g/100cc
2.	Ethanol	Column 2:	4.45698	0.0523	g/100cc
3.	n-Propanol	Column 1:	45.35659	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.21875	1.0000	g/100cc

W

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.100 FN02271802
 Laboratory : Meridian
 Injection Date : Nov 29, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

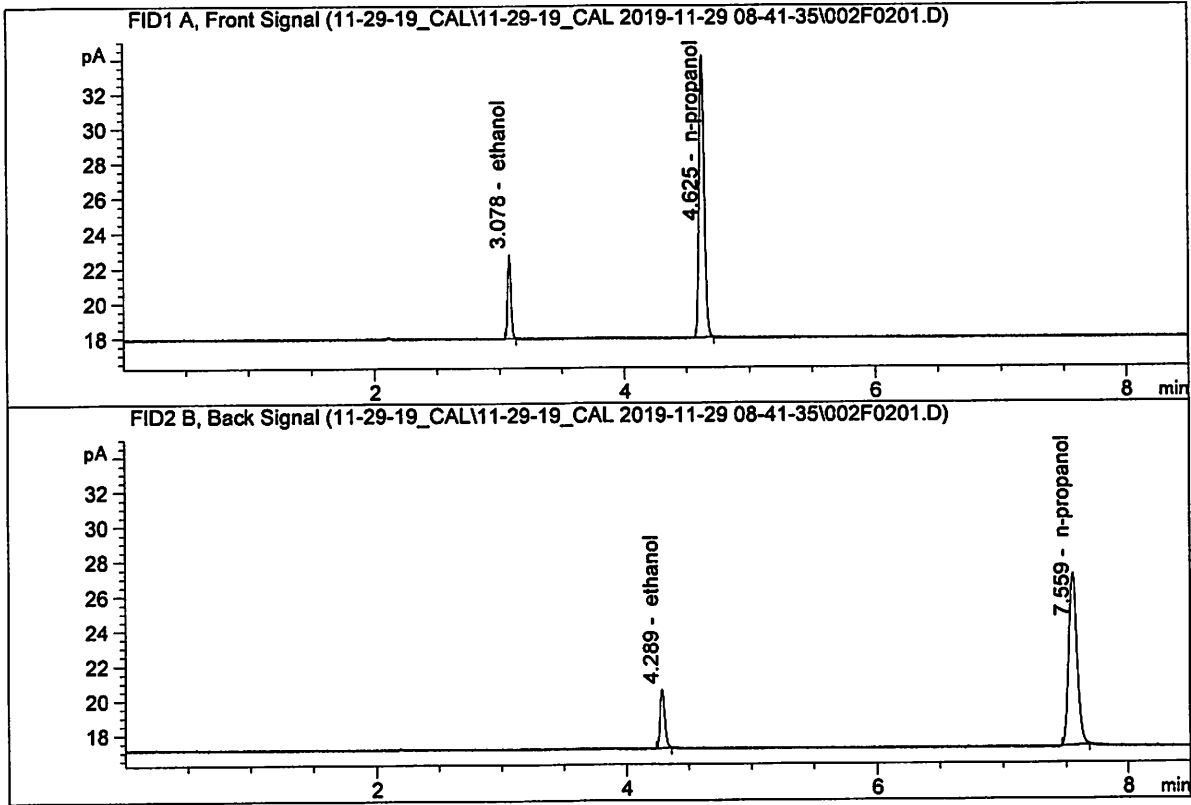


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	8.81372	0.0998	g/100cc
2.	Ethanol	Column 2:	9.04277	0.0995	g/100cc
3.	n-Propanol	Column 1:	46.09383	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.70168	1.0000	g/100cc

Handwritten signature

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.200 FN06231704
 Laboratory : Meridian
 Injection Date : Nov 29, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014 -CN11041167

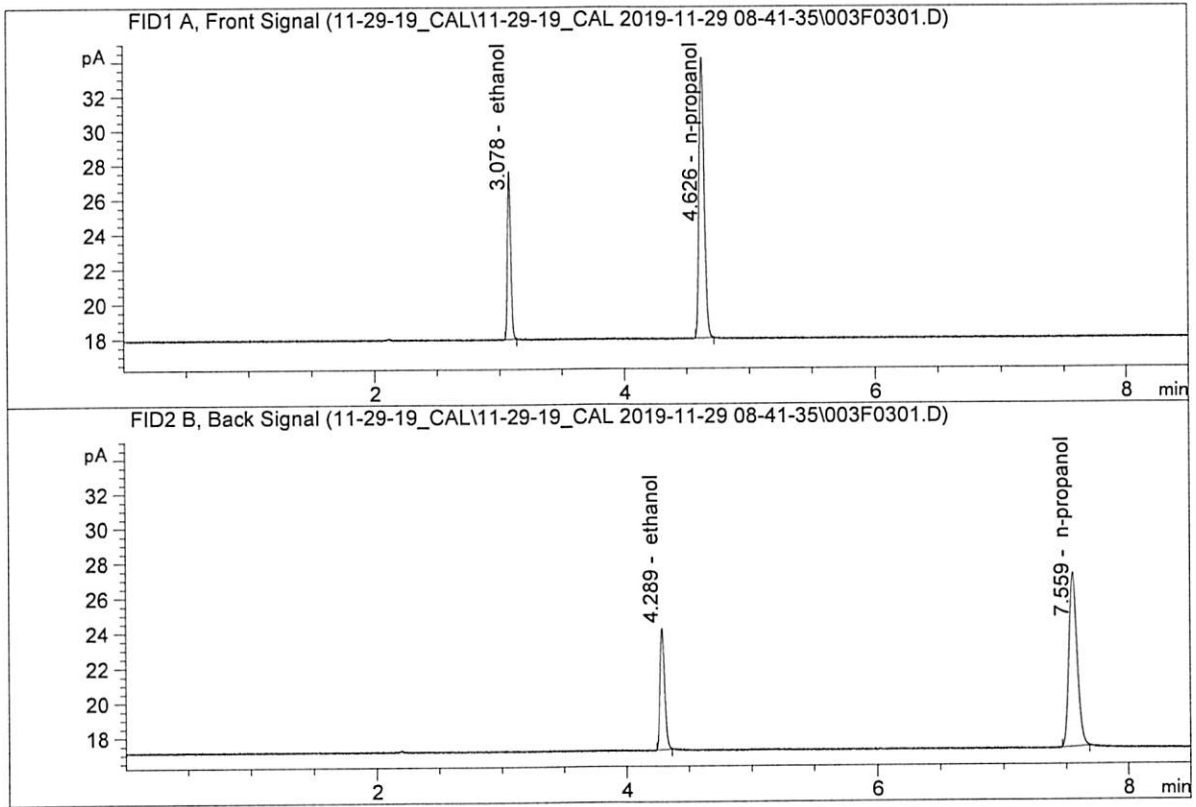


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	17.73868	0.1992	g/100cc
2.	Ethanol	Column 2:	18.43505	0.1975	g/100cc
3.	n-Propanol	Column 1:	46.20026	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.67413	1.0000	g/100cc

Handwritten signature

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.300 FN07311804
 Laboratory : Meridian
 Injection Date : Nov 29, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

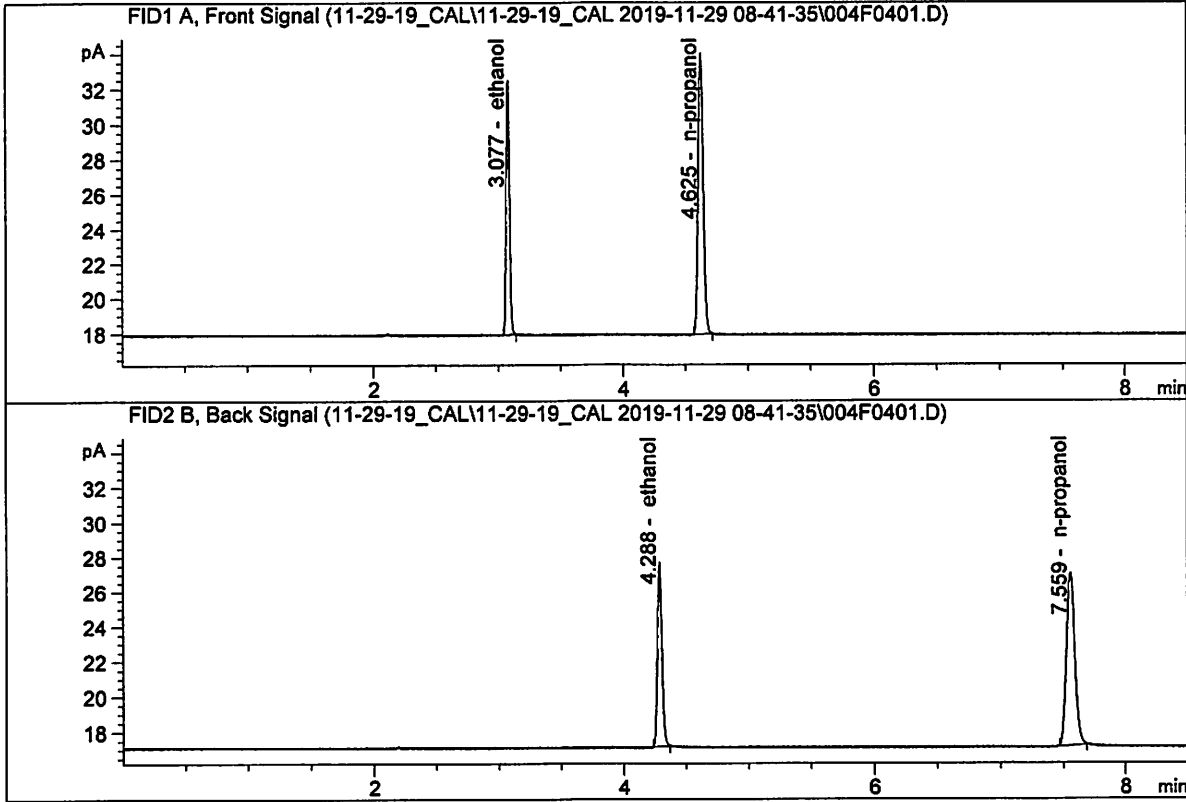


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	26.62050	0.3007	g/100cc
2.	Ethanol	Column 2:	27.88322	0.2996	g/100cc
3.	n-Propanol	Column 1:	45.82462	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.07686	1.0000	g/100cc

W

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.500 FN08031602
 Laboratory : Meridian
 Injection Date : Nov 29, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

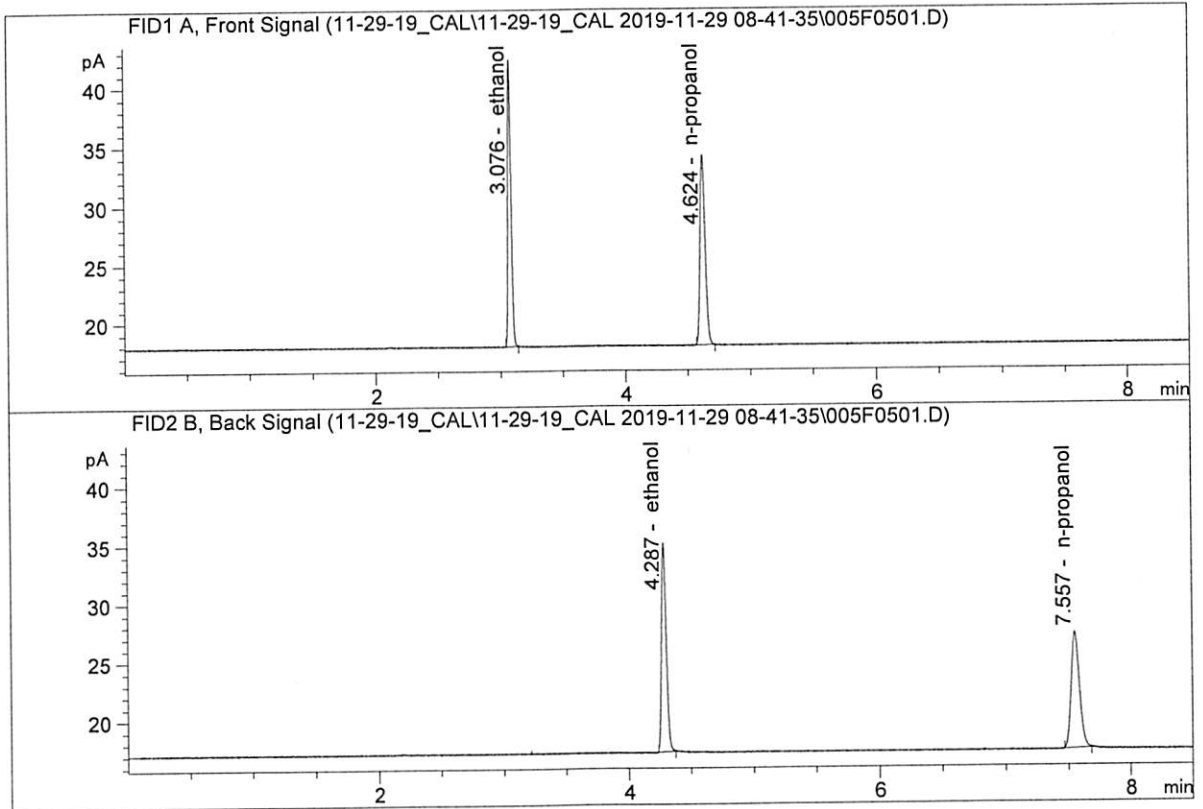


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	44.55405	0.4999	g/100cc
2.	Ethanol	Column 2:	47.09054	0.5011	g/100cc
3.	n-Propanol	Column 1:	46.05164	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.19093	1.0000	g/100cc

Handwritten signature

ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STANDARD BLANK
 Laboratory : Meridian
 Injection Date : Nov 29, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

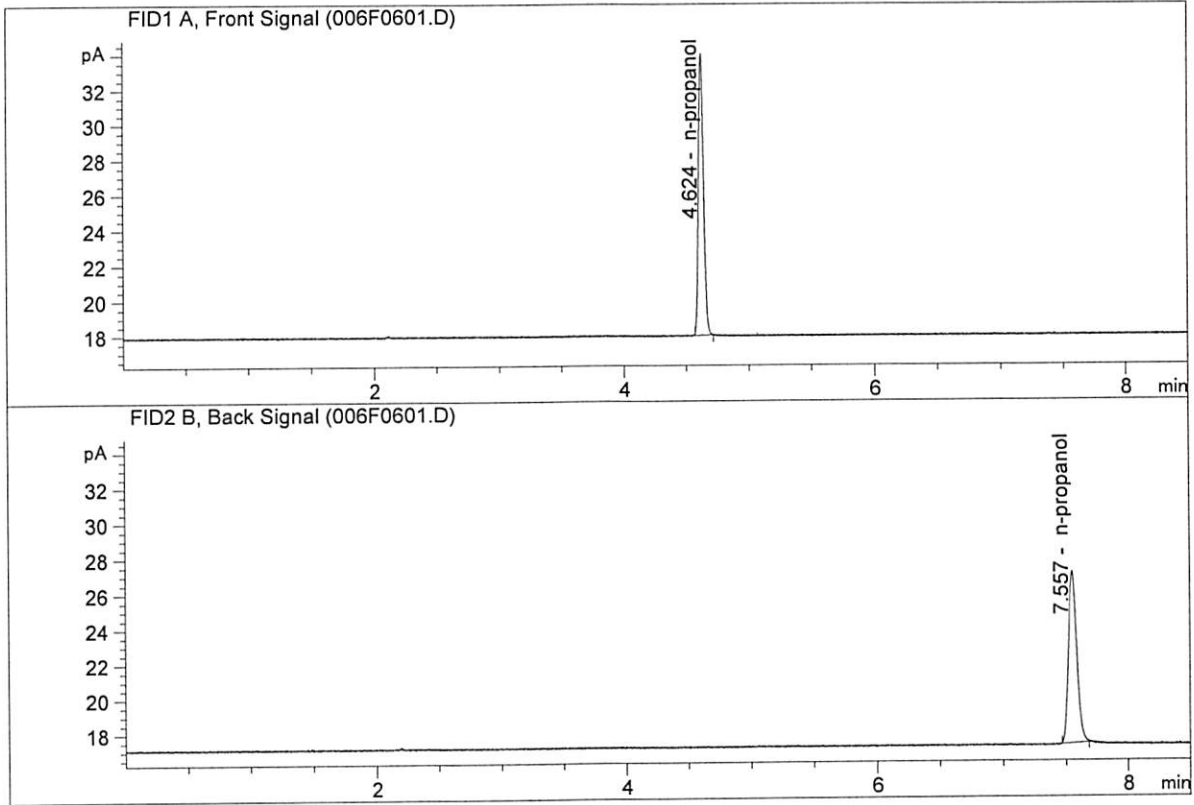

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	45.66352	1.0000	g/100cc
4.	n-Propanol	Column 2:	46.94871	1.0000	g/100cc

W

S a m p l e S u m m a r y


Sequence table: C:\Chem32\1\Data\11-29-19_CAL\11-29-19_CAL 2019-11-29 08-41-35\11-29-19_CAL.S
 Data directory path: C:\Chem32\1\Data\11-29-19_CAL\11-29-19_CAL 2019-11-29 08-41-35\
 Logbook: C:\Chem32\1\Data\11-29-19_CAL\11-29-19_CAL 2019-11-29 08-41-35\11-29-19_CAL.LOG
 Sequence start: 11/29/2019 8:56:13 AM
 Sequence Operator: SYSTEM
 Operator: SYSTEM

Method file name: C:\Chem32\1\Data\11-29-19_CAL\11-29-19_CAL 2019-11-29 08-41-35\ALCOHOL.M

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #	# Cmp
1	1	1	0.050 FN05211804	-	1.0000	001F0101.D	*	4
2	2	1	0.100 FN02271802	-	1.0000	002F0201.D	*	4
3	3	1	0.200 FN06231704	-	1.0000	003F0301.D	*	4
4	4	1	0.300 FN07311804	-	1.0000	004F0401.D	*	4
5	5	1	0.500 FN08031602	-	1.0000	005F0501.D	*	4
6	6	1	INTERNAL STANDAR	-	1.0000	006F0601.D		2

ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STD BLK 1
 Laboratory : Meridian
 Injection Date : Dec 5, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

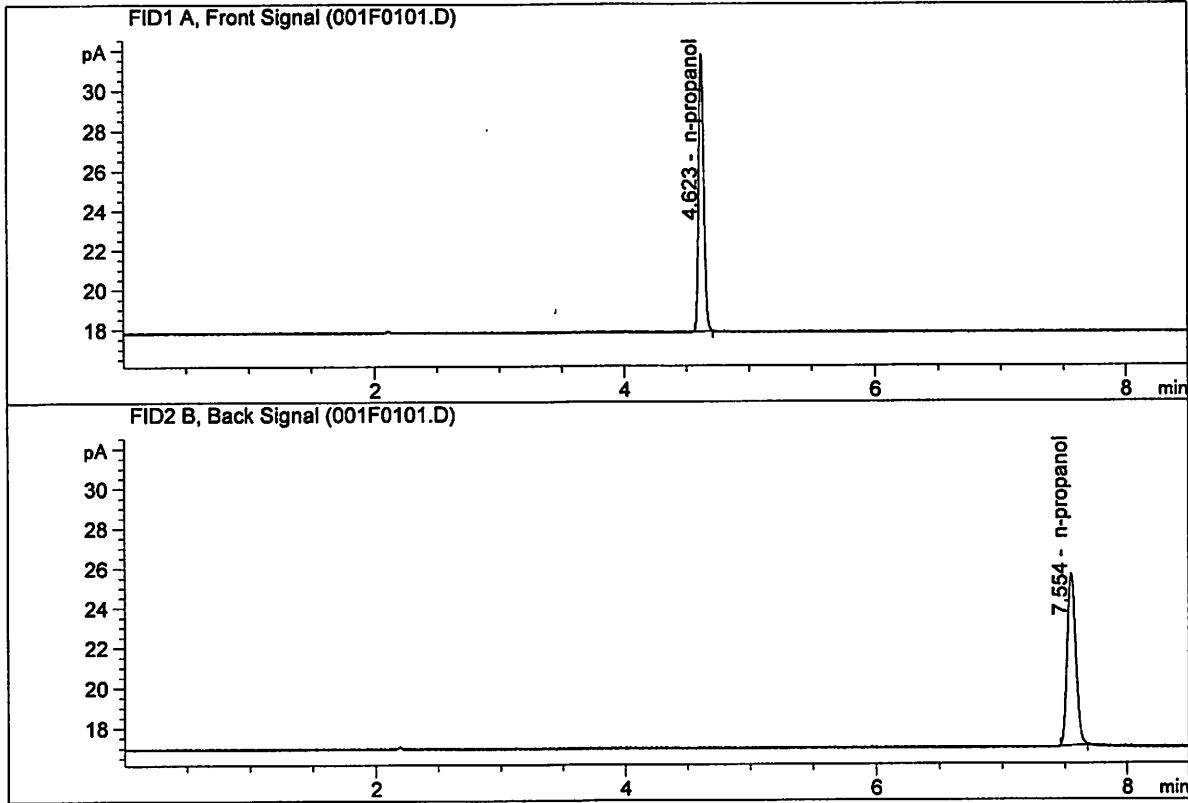


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	39.44083	1.0000	g/100cc
4.	n-Propanol	Column 2:	41.11308	1.0000	g/100cc

W

ISP Forensic Services Blood Alcohol Report

Sample Name : MIX VOL FN06041502
 Laboratory : Meridian
 Injection Date : Dec 5, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

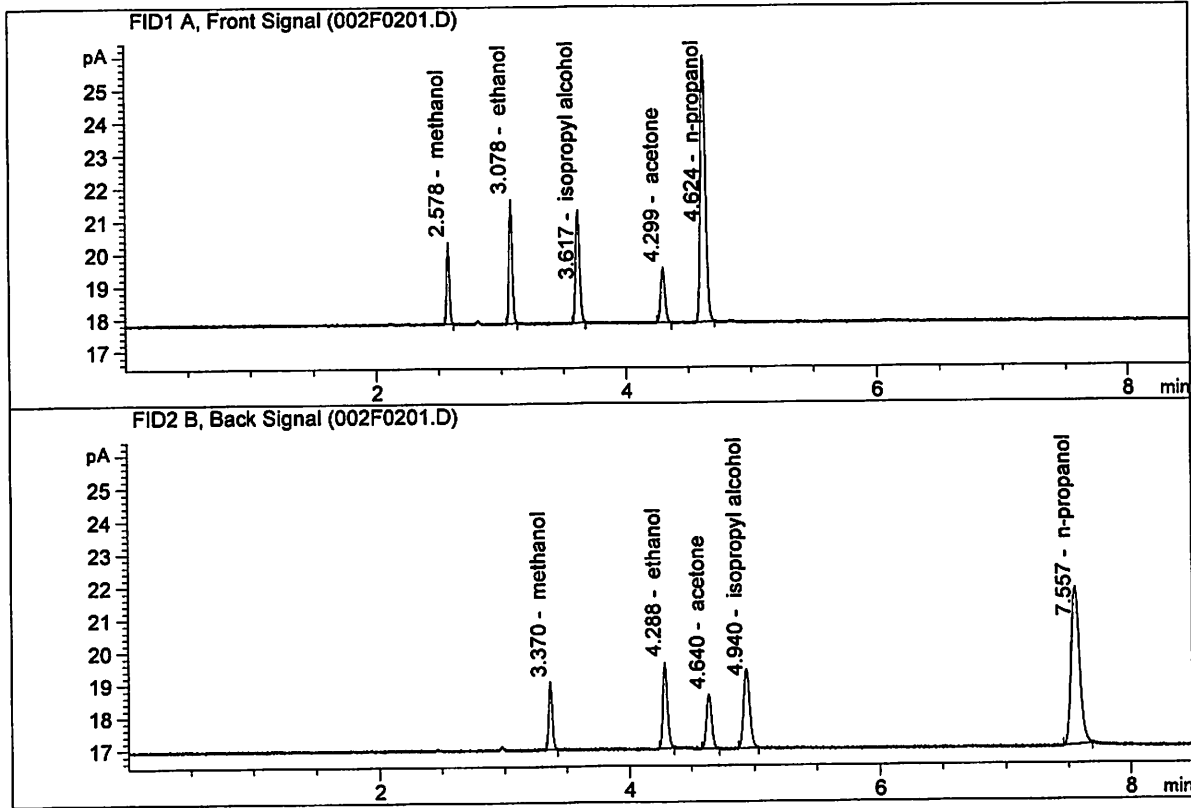

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	6.75257	0.1534	g/100cc
2.	Ethanol	Column 2:	6.98239	0.1542	g/100cc
3.	n-Propanol	Column 1:	22.88158	1.0000	g/100cc
4.	n-Propanol	Column 2:	23.30162	1.0000	g/100cc

N

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC1-1

Analysis Date(s): 05 Dec 2019

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.0808	0.0818	0.0010	0.0813	0.0810	
(g/100cc)	0.0803	0.0814	0.0011	0.0808		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: Alcohol.m
Hamilton Auto-Dilutor Serial Number: ML600HC11378

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.081	0.076	0.086	0.005

	Reported Result	
	0.081	

Calibration and control data are stored centrally.

W


Revision: 1

Issue Date: 01/04/2019

Issuing Authority: Quality Manager

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-1-A
 Laboratory : Meridian
 Injection Date : Dec 5, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

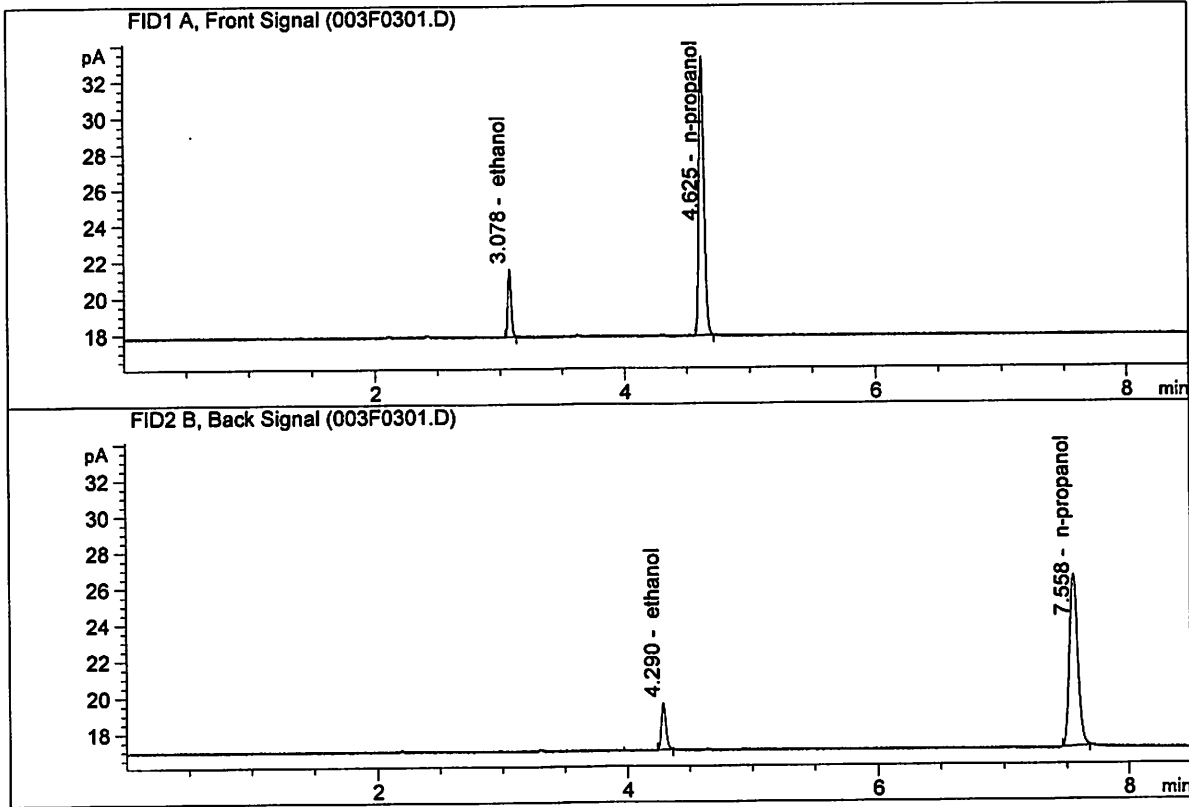


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	6.76536	0.0808	g/100cc
2.	Ethanol	Column 2:	6.96093	0.0818	g/100cc
3.	n-Propanol	Column 1:	43.81967	1.0000	g/100cc
4.	n-Propanol	Column 2:	45.23341	1.0000	g/100cc

W

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-1-B
 Laboratory : Meridian
 Injection Date : Dec 5, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

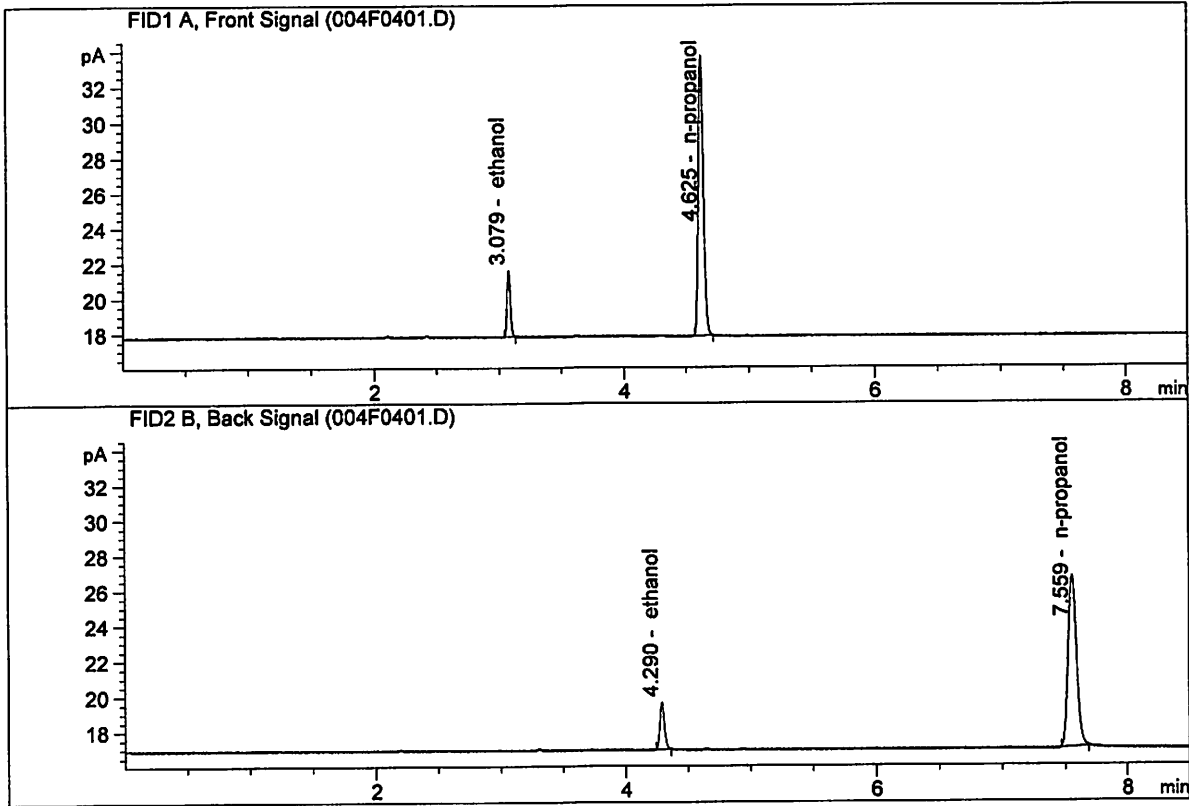

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	6.89878	0.0803	g/100cc
2.	Ethanol	Column 2:	7.10301	0.0814	g/100cc
3.	n-Propanol	Column 1:	45.00264	1.0000	g/100cc
4.	n-Propanol	Column 2:	46.40219	1.0000	g/100cc

W

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: 0.08 FN04171701

Analysis Date(s): 05 Dec 2019

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.0808	0.0815	0.0007	0.0811	0.0811	
(g/100cc)	0.0809	0.0814	0.0005	0.0811		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: Alcohol.m
Hamilton Auto-Dilutor Serial Number: ML600HC11378

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%


Overall Mean (g/100cc)	Low	High	5% of Mean
0.081	0.076	0.086	0.005

	Reported Result	
	0.081	

Calibration and control data are stored centrally.

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.08 FN04171701-A
 Laboratory : Meridian
 Injection Date : Dec 5, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

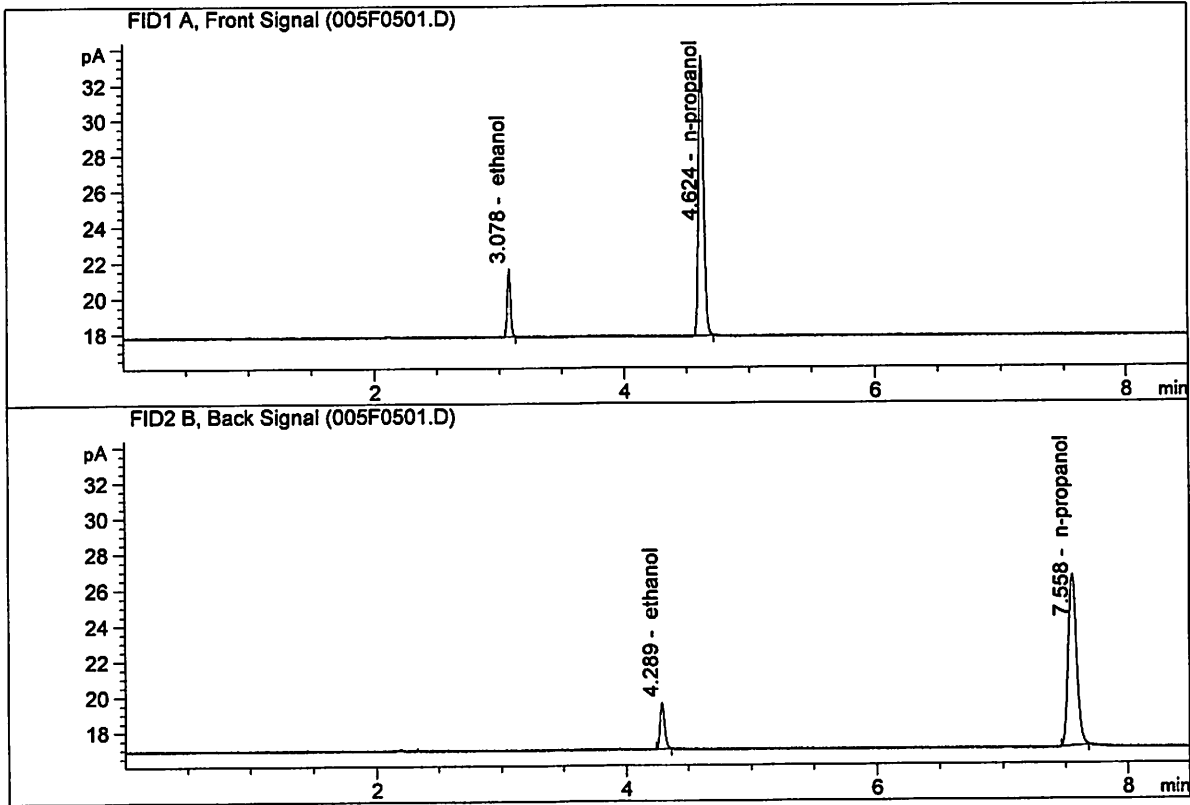


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	6.90173	0.0808	g/100cc
2.	Ethanol	Column 2:	7.06795	0.0815	g/100cc
3.	n-Propanol	Column 1:	44.74257	1.0000	g/100cc
4.	n-Propanol	Column 2:	46.10887	1.0000	g/100cc

W

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.08 FN04171701-B
 Laboratory : Meridian
 Injection Date : Dec 5, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

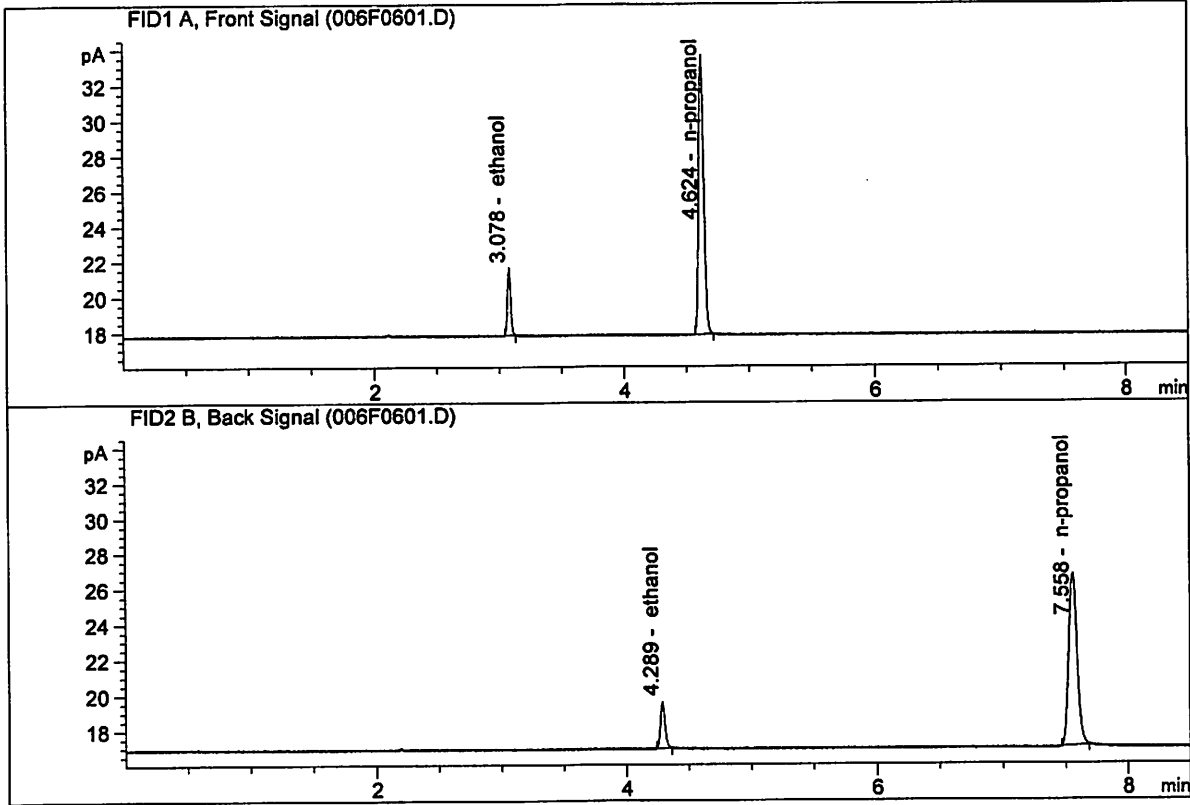

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	6.94512	0.0809	g/100cc
2.	Ethanol	Column 2:	7.09785	0.0814	g/100cc
3.	n-Propanol	Column 1:	44.91950	1.0000	g/100cc
4.	n-Propanol	Column 2:	46.40028	1.0000	g/100cc

av

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC2-1

Analysis Date(s): 05 Dec 2019

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.1955	0.1952	0.0003	0.1953	0.1959	
(g/100cc)	0.1967	0.1964	0.0003	0.1965		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: Alcohol.m
Hamilton Auto-Dilutor Serial Number: ML600HC11378

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%


Overall Mean (g/100cc)	Low	High	5% of Mean
0.195	0.185	0.205	0.010

	Reported Result	
	0.195	

Calibration and control data are stored centrally.

ISP Forensic Services Blood Alcohol Report

Sample Name : QC2-1-A
 Laboratory : Meridian
 Injection Date : Dec 5, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

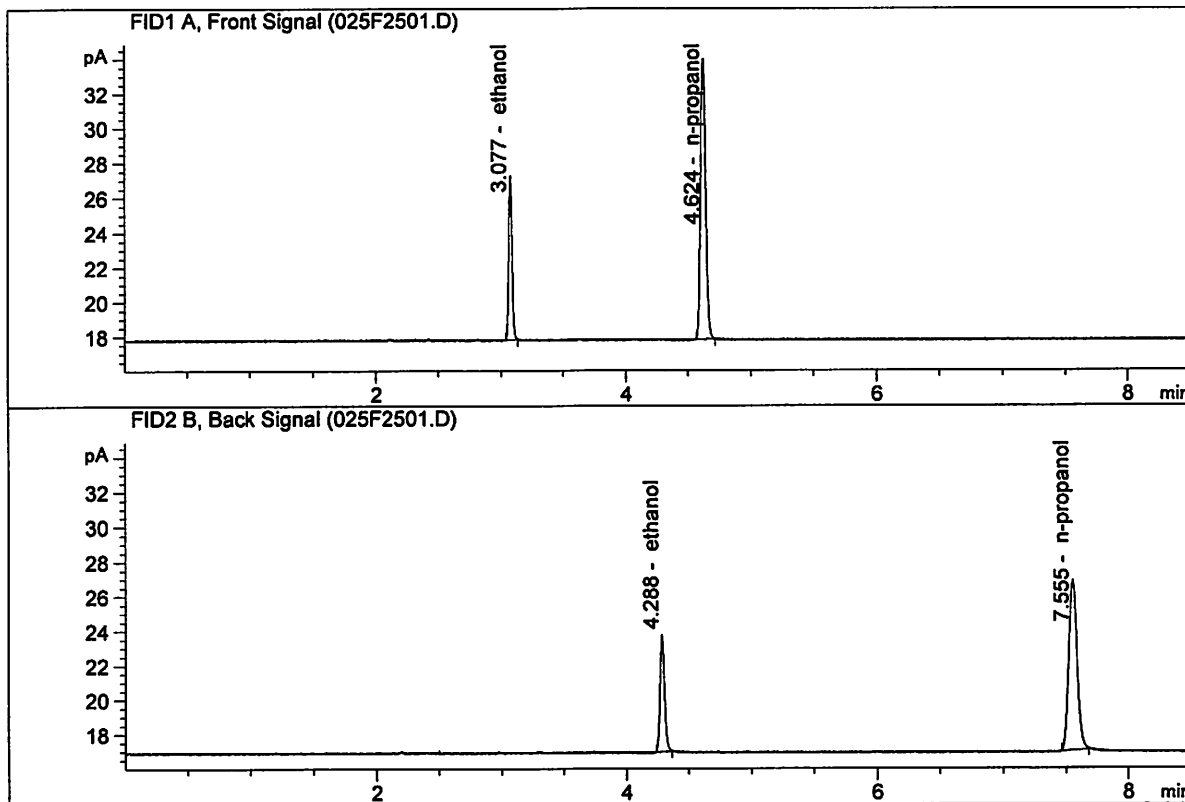


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	17.33387	0.1955	g/100cc
2.	Ethanol	Column 2:	18.04504	0.1952	g/100cc
3.	n-Propanol	Column 1:	46.00539	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.23572	1.0000	g/100cc

W

ISP Forensic Services Blood Alcohol Report

Sample Name : QC2-1-B
 Laboratory : Meridian
 Injection Date : Dec 5, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

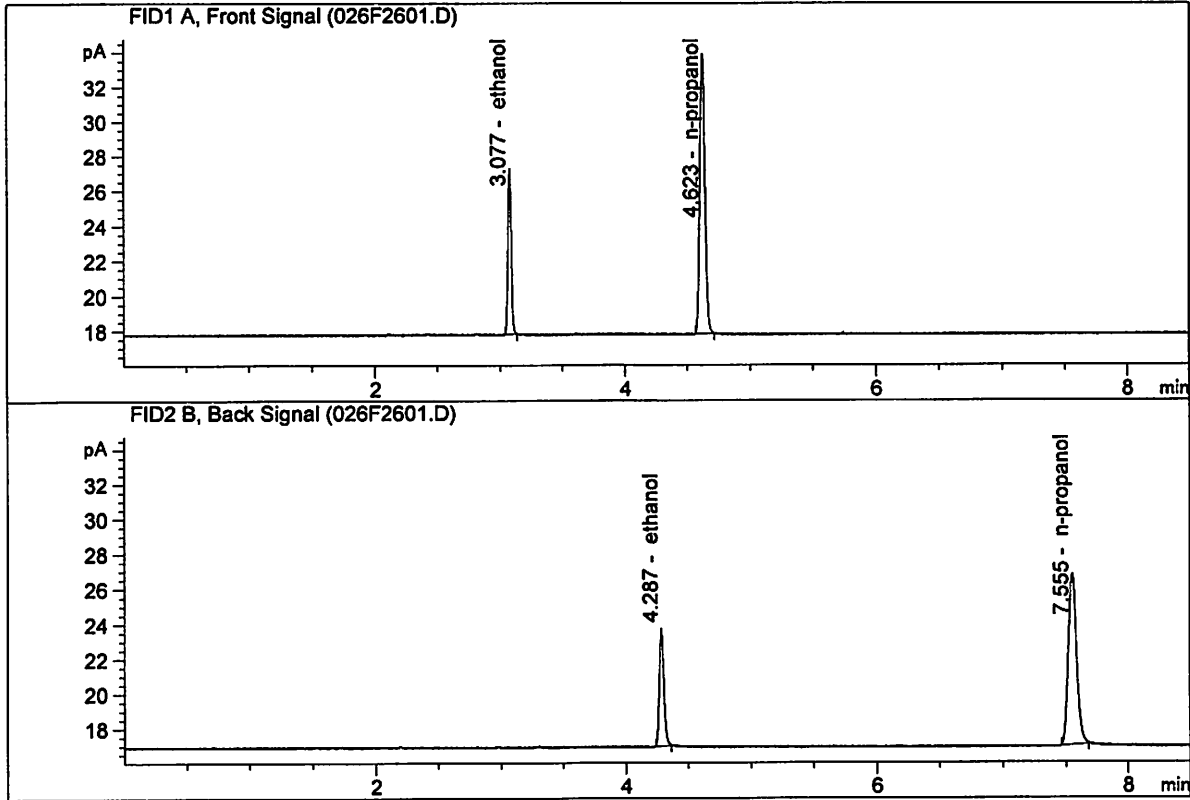

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	17.31893	0.1967	g/100cc
2.	Ethanol	Column 2:	18.01380	0.1964	g/100cc
3.	n-Propanol	Column 1:	45.67154	1.0000	g/100cc
4.	n-Propanol	Column 2:	46.85586	1.0000	g/100cc

W

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC1-2

Analysis Date(s): 05 Dec 2019

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.0805	0.0813	0.0008	0.0809	0.0810	
(g/100cc)	0.0806	0.0816	0.0010	0.0811		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: Alcohol.m
Hamilton Auto-Dilutor Serial Number: ML600HC11378

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%


Overall Mean (g/100cc)	Low	High	5% of Mean
0.081	0.076	0.086	0.005

	Reported Result	
	0.081	

Calibration and control data are stored centrally.

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-2-A
 Laboratory : Meridian
 Injection Date : Dec 5, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

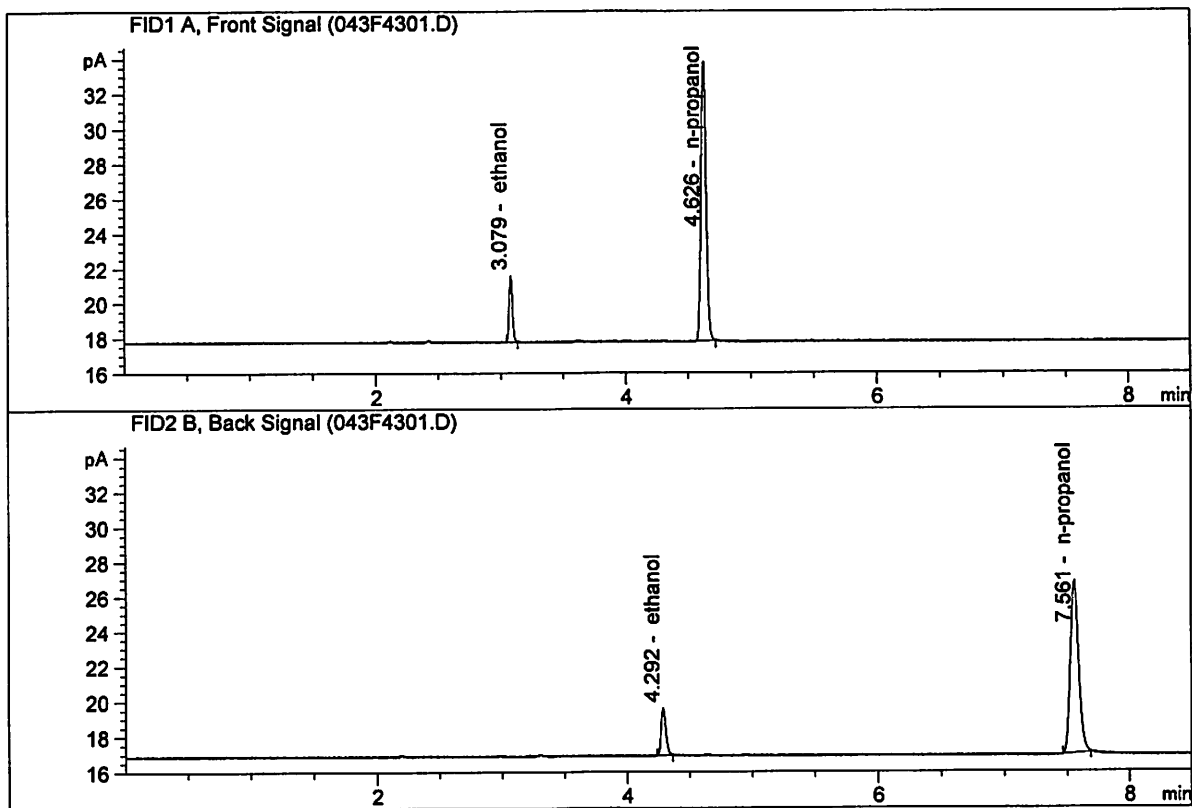


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.01451	0.0805	g/100cc
2.	Ethanol	Column 2:	7.18879	0.0813	g/100cc
3.	n-Propanol	Column 1:	45.60191	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.01132	1.0000	g/100cc

W

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-2-B
 Laboratory : Meridian
 Injection Date : Dec 5, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

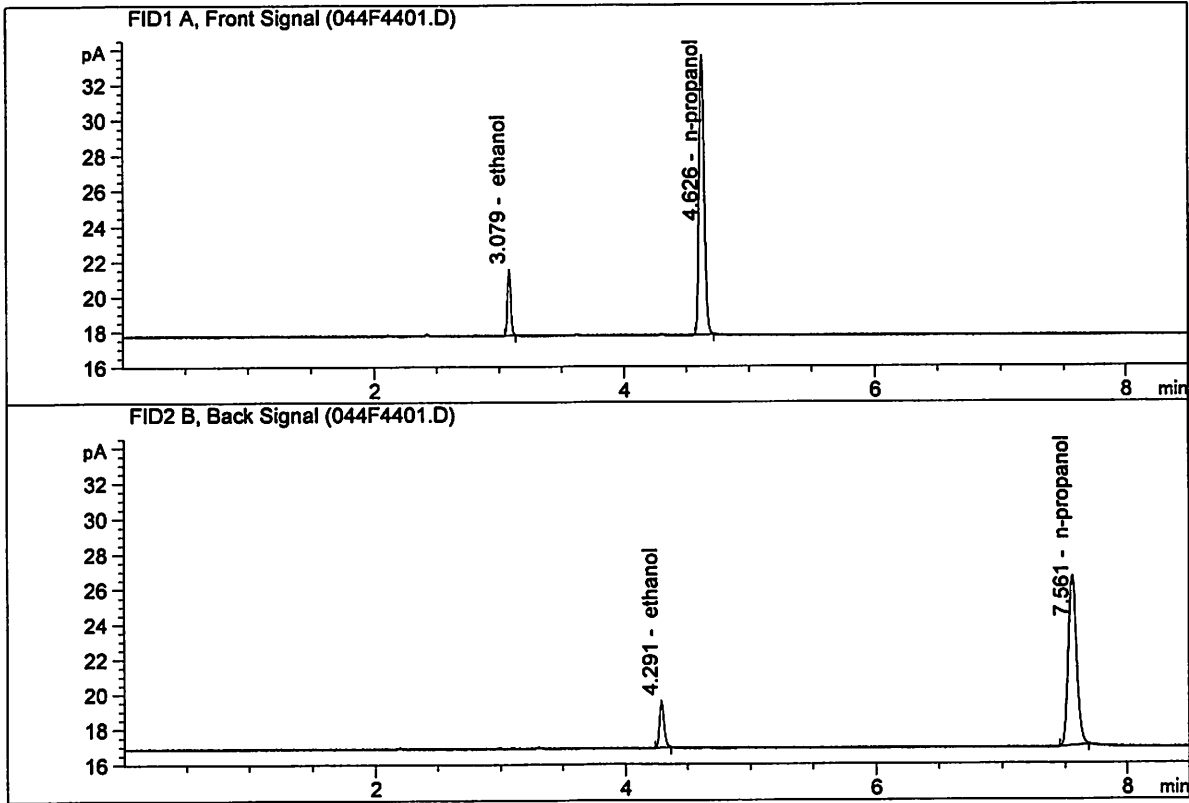


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	6.93564	0.0806	g/100cc
2.	Ethanol	Column 2:	7.13830	0.0816	g/100cc
3.	n-Propanol	Column 1:	45.06354	1.0000	g/100cc
4.	n-Propanol	Column 2:	46.49244	1.0000	g/100cc

W

ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STD BLK
 Laboratory : Meridian
 Injection Date : Dec 5, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

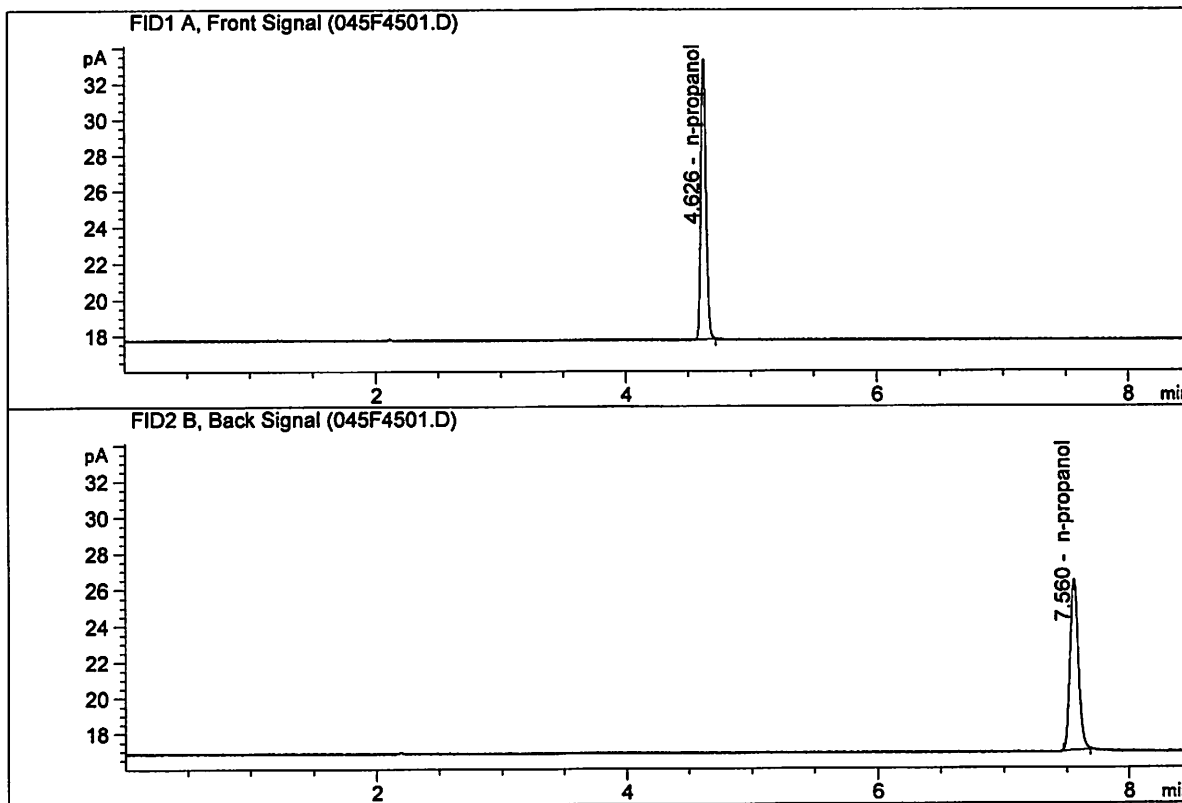

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	44.17079	1.0000	g/100cc
4.	n-Propanol	Column 2:	45.35441	1.0000	g/100cc

W

Sample Summary

Sequence table: C:\Chem32\1\Data\12-05-19_SAMPLES\12-05-19_SAMPLES 2019-12-05 10-18-56\12-05-19_SAMPLES.S
 Data directory path: C:\Chem32\1\Data\12-05-19_SAMPLES\12-05-19_SAMPLES 2019-12-05 10-18-56\
 Logbook: C:\Chem32\1\Data\12-05-19_SAMPLES\12-05-19_SAMPLES 2019-12-05 10-18-56\12-05-19_SAMPLES.LOG
 Sequence start: 12/5/2019 10:33:40 AM
 Sequence Operator: SYSTEM
 Operator: SYSTEM
 Method file name: C:\Chem32\1\Data\12-05-19_SAMPLES\12-05-19_SAMPLES 2019-12-05 10-18-56\ALCOHOL.M

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip. * Dilution	File name	Cal #	# Cmp
1	1	1	INTERNAL STD BLK	-	1.0000	001F0101.D		2
2	2	1	MIX VOL FN060415	-	1.0000	002F0201.D		10
3	3	1	QC1-1-A	-	1.0000	003F0301.D		4
4	4	1	QC1-1-B	-	1.0000	004F0401.D		4
5	5	1	0.08 FN04171701-	-	1.0000	005F0501.D		4
6	6	1	0.08 FN04171701-	-	1.0000	006F0601.D		4
7	7	1	M2019-5366-1-A	-	1.0000	007F0701.D		4
8	8	1	M2019-5366-1-B	-	1.0000	008F0801.D		4
9	9	1	M2019-5367-1-A	-	1.0000	009F0901.D		4
10	10	1	M2019-5367-1-B	-	1.0000	010F1001.D		4
11	11	1	M2019-5368-1-A	-	1.0000	011F1101.D		4
12	12	1	M2019-5368-1-B	-	1.0000	012F1201.D		4
13	13	1	M2019-5369-1-A	-	1.0000	013F1301.D		4
14	14	1	M2019-5369-1-B	-	1.0000	014F1401.D		4
15	15	1	M2019-5404-1-A	-	1.0000	015F1501.D		4
16	16	1	M2019-5404-1-B	-	1.0000	016F1601.D		4
17	17	1	P2019-3548-1-A	-	1.0000	017F1701.D		5
18	18	1	P2019-3548-1-B	-	1.0000	018F1801.D		6
19	19	1	P2019-3565-1-A	-	1.0000	019F1901.D		4
20	20	1	P2019-3565-1-B	-	1.0000	020F2001.D		4
21	21	1	P2019-3566-1-A	-	1.0000	021F2101.D		4
22	22	1	P2019-3566-1-B	-	1.0000	022F2201.D		4
23	23	1	P2019-3567-1-A	-	1.0000	023F2301.D		4
24	24	1	P2019-3567-1-B	-	1.0000	024F2401.D		4
25	25	1	QC2-1-A	-	1.0000	025F2501.D		4
26	26	1	QC2-1-B	-	1.0000	026F2601.D		4
27	27	1	P2019-3572-1-A	-	1.0000	027F2701.D		4
28	28	1	P2019-3572-1-B	-	1.0000	028F2801.D		4
29	29	1	P2019-3584-1-A	-	1.0000	029F2901.D		2
30	30	1	P2019-3584-1-B	-	1.0000	030F3001.D		2
31	31	1	P2019-3588-1-A	-	1.0000	031F3101.D		4
32	32	1	P2019-3588-1-B	-	1.0000	032F3201.D		4
33	33	1	P2019-3602-1-A	-	1.0000	033F3301.D		4
34	34	1	P2019-3602-1-B	-	1.0000	034F3401.D		4
35	35	1	P2019-3603-1-A	-	1.0000	035F3501.D		4
36	36	1	P2019-3603-1-B	-	1.0000	036F3601.D		4
37	37	1	P2019-3605-1-A	-	1.0000	037F3701.D		4
38	38	1	P2019-3605-1-B	-	1.0000	038F3801.D		4
39	39	1	P2019-3614-1-A	-	1.0000	039F3901.D		4
40	40	1	P2019-3614-1-B	-	1.0000	040F4001.D		4
41	41	1	P2019-3615-1-A	-	1.0000	041F4101.D		2
42	42	1	P2019-3615-1-B	-	1.0000	042F4201.D		2
43	43	1	QC1-2-A	-	1.0000	043F4301.D		4

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #
44	44	1	QC1-2-B	-	1.0000	044F4401.D	4
45	45	1	INTERNAL STD BLK	-	1.0000	045F4501.D	2

Method file name: C:\Chem32\1\Data\12-05-19_SAMPLES\12-05-19_SAMPLES 2019-12-05 10-18-56 \SHUTDOWN.M

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #
46	46	1	EMPTY	-	1.0000	046F4601.D	0

