

I reviewed and approved central data packet for worklist 4530 on 9/21/2020 at 11:00 am.

Due to a software issue, I was unable to stamp it electronically at the time.

Galina Giso

9/23/2020

Quantitative Analysis for Ethanol & Qualitative Analysis for Other Volatiles

Analytical Method(s): 1.0

Device: Hamilton MICROLAB Liquid Processor/Dilutor Serial Number: ML600HC11378

Volatiles Quality Assurance Controls Run Date(s): 9/18/20-9/19/20

Calibration Date(s): 9/18/20

| Control level | Expiration | Lot # | Target Value | Acceptable Range | Overall Results |
|---------------------------------|------------|--------------|-----------------|------------------|---|
| Level 1 | Jul-23 | 1907006 | 0.0764 | 0.0688-0.0840 | 0.0735 g/100cc 0.0747 g/100cc g/100cc |
| Level 2 | Mar-22 | 1803028 | 0.2035 | 0.1832-0.2238 | 0.1984 g/100cc g/100cc |
| Multi-Component mixture: | | Lot # | Column 1 | Column 2 | ok |
| Curve Fit: | | 0.99998 | FN07101701 | 0.99992 | |

Ethanol Calibration Reference Material

| Calibrator level | Target Value | Acceptable Range | Column 1 | Column 2 | Precision | Mean |
|------------------|--------------|------------------|----------|----------|-----------|---------|
| 50 | 0.050 | 0.045 - 0.055 | 0.0506 | 0.0521 | 0.0015 | 0.0513 |
| 100 | 0.100 | 0.090 - 0.110 | 0.1002 | 0.1000 | 0.0002 | 0.1001 |
| 200 | 0.200 | 0.180 - 0.220 | 0.2000 | 0.1990 | 0.001 | 0.1995 |
| 300 | 0.300 | 0.270 - 0.330 | | | 0 | #DIV/0! |
| 400 | 0.400 | 0.360 - 0.440 | 0.2983 | 0.2967 | 0.0016 | 0.2975 |
| 500 | 0.500 | 0.450 - 0.550 | 0.5009 | 0.5022 | 0.0013 | 0.5015 |


Aqueous Controls

| Control level | Target Value | Acceptable Range | Overall Results |
|---------------|--------------|------------------|-----------------|
| 80 | 0.080 | 0.076 - 0.084 | 0.080 g/100cc |

JG

Worklist: 4530

| LAB CASE | ITEM | ITEM TYPE | DESCRIPTION |
|------------|------|-----------|-----------------------|
| M2020-3449 | 2 | BCK | Alcohol Analysis |
| M2020-3510 | 1 | BCK | BATS Proficiency Test |
| M2020-3538 | 1 | BCK | Alcohol Analysis |
| M2020-3539 | 1 | BCK | Alcohol Analysis |
| M2020-3584 | 1 | BCK | Alcohol Analysis |
| M2020-3585 | 1 | BCK | Alcohol Analysis |
| M2020-3598 | 1 | BCK | Alcohol Analysis |
| M2020-3632 | 1 | BCK | Alcohol Analysis |
| M2020-3642 | 1 | BCK | Alcohol Analysis |
| M2020-3660 | 1 | BCK | Alcohol Analysis |
| M2020-3661 | 1 | BCK | Alcohol Analysis |
| M2020-3668 | 1 | BCK | Alcohol Analysis |
| M2020-3688 | 1 | BCK | Alcohol Analysis |
| M2020-3689 | 1 | BCK | Alcohol Analysis |
| M2020-3701 | 1 | BCK | Alcohol Analysis |
| P2020-2169 | 2 | BCK | Alcohol Analysis |

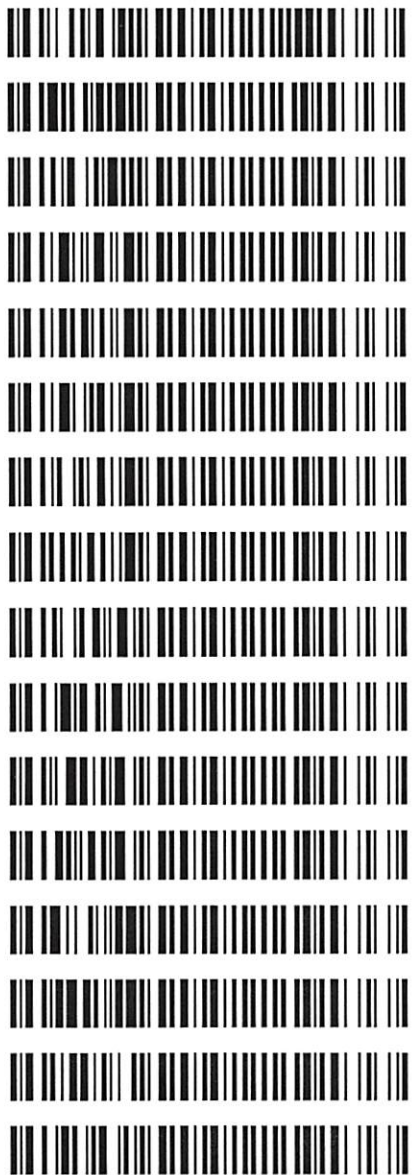

jc

=====
Calibration Table
=====

General Calibration Setting

Calib. Data Modified : Friday, September 18, 2020 3:23:20 PM
Signals calculated separately : No

Rel. Reference Window : 0.000 %
Abs. Reference Window : 0.100 min
Rel. Non-ref. Window : 0.000 %
Abs. Non-ref. Window : 0.100 min
Uncalibrated Peaks : not reported
Partial Calibration : Yes, identified peaks are recalibrated
Correct All Ret. Times : No, only for identified peaks

Curve Type : Linear
Origin : Ignored
Weight : Equal

Recalibration Settings : Average all calibrations
Average Response :
Average Retention Time : Floating Average New 75%

Calibration Report Options :
Printout of recalibrations within a sequence:
Calibration Table after Recalibration
Normal Report after Recalibration
If the sequence is done with bracketing:
Results of first cycle (ending previous bracket)

Default Sample ISTD Information (if not set in sample table):
ISTD ISTD Amount Name # [g/100cc]
-----|-----|-----
1 1.00000 n-propanol
2 1.00000 n-propanol

Signal Details

Signal 1: FID1 A, Front Signal
Signal 2: FID2 B, Back Signal

Overview Table

jc

| RT | Stg | Lvl | Amount | Area | Rsp. Factor | Ref | ISTD | # | Compound |
|-------|-----|-----|------------|----------|-------------|-----|------|---|-------------------|
| 2.586 | 1 | 1 | 1.00000 | 3.69669 | 2.70512e-1 | No | No | 1 | methanol |
| 2.809 | 1 | 1 | 1.00000 | 4.26100 | 2.34687e-1 | No | No | 2 | Acetaldehyde |
| 2.977 | 2 | 1 | 1.00000 | 4.26100 | 2.34687e-1 | No | No | 2 | Acetaldehyde |
| 3.075 | 1 | 1 | 5.00000e-2 | 4.59217 | 1.08881e-2 | No | No | 1 | ethanol |
| 3.388 | 2 | 1 | 1.00000 | 4.26062 | 2.34707e-1 | No | No | 2 | methanol |
| 3.628 | 1 | 1 | 1.00000 | 9.73055 | 1.02769e-1 | No | No | 1 | isopropyl alcohol |
| 4.285 | 2 | 1 | 5.00000e-2 | 4.68252 | 1.06780e-2 | No | No | 2 | ethanol |
| 4.308 | 1 | 1 | 1.00000 | 6.49940 | 1.53860e-1 | No | No | 1 | acetone |
| 4.620 | 1 | 1 | 1.00000 | 47.73816 | 2.09476e-2 | No | Yes | 1 | n-propanol |
| 4.661 | 2 | 1 | 1.00000 | 6.89301 | 1.45075e-1 | No | No | 2 | acetone |
| 4.969 | 2 | 1 | 1.00000 | 10.70642 | 9.34019e-2 | No | No | 2 | isopropyl alcohol |
| 7.550 | 2 | 1 | 1.00000 | 49.51909 | 2.01942e-2 | No | Yes | 2 | n-propanol |
| | | | | 48.45788 | 2.06365e-2 | | | | |
| | | | | 48.32198 | 2.06945e-2 | | | | |
| | | | | 49.01604 | 2.04015e-2 | | | | |
| | | | | 48.37467 | 2.06720e-2 | | | | |

Peak Sum Table





No Entries in table

41 Warnings or Errors (10 first messages follow) :

Warning : Curve requires more calibration points, (methanol)
 Warning : Curve requires more calibration points, at 2.586 min, signal 1
 Warning : Curve requires more calibration points, at 2.809 min, signal 1
 Warning : Curve requires more calibration points, at 2.977 min, signal 2
 Warning : Curve requires more calibration points, at 3.388 min, signal 2
 Warning : Curve requires more calibration points, at 3.628 min, signal 1
 Warning : Curve requires more calibration points, at 4.308 min, signal 1
 Warning : Curve requires more calibration points, at 4.62 min, signal 1
 Warning : Curve requires more calibration points, at 4.661 min, signal 2
 Warning : Curve requires more calibration points, at 4.969 min, signal 2


0c

=====
Calibration Curves
=====

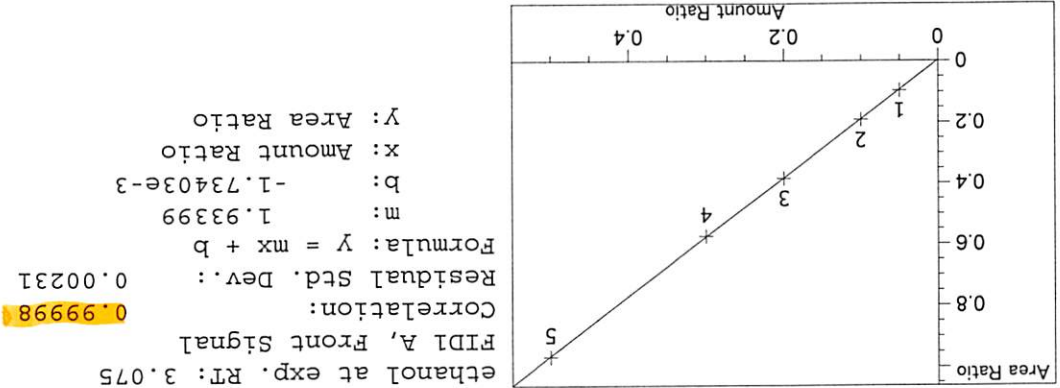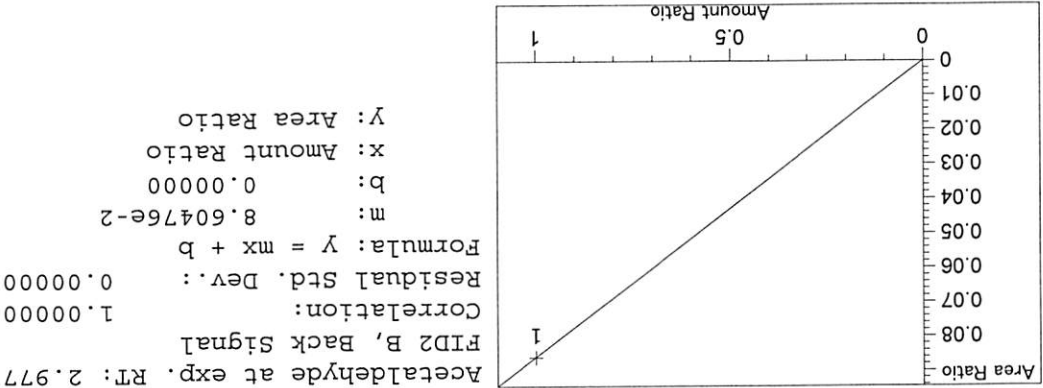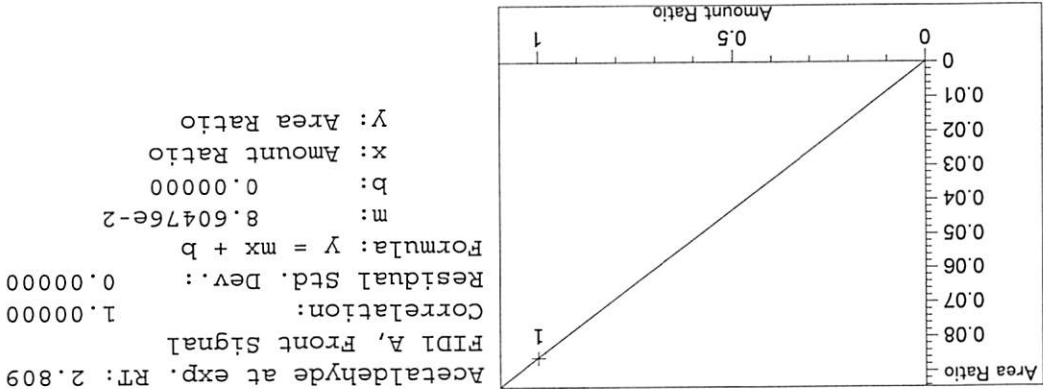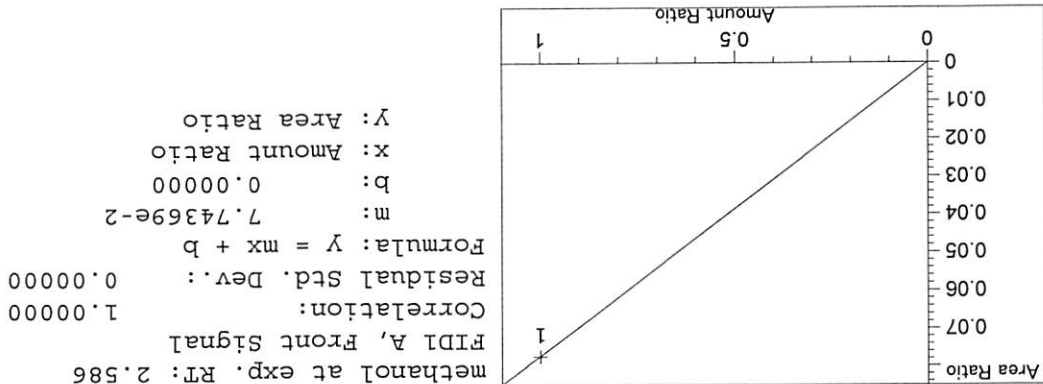


jc


methanol at exp. RT: 3.388
 FID2 B, Back Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $Y = mx + b$
 m: 8.60401e-2
 b: 0.00000
 x: Amount Ratio
 Y: Area Ratio

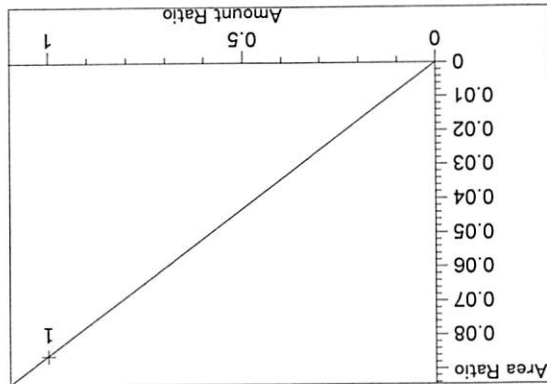


isopropyl alcohol at exp. RT: 3.628
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $Y = mx + b$
 m: 2.03832e-1
 b: 0.00000
 x: Amount Ratio
 Y: Area Ratio

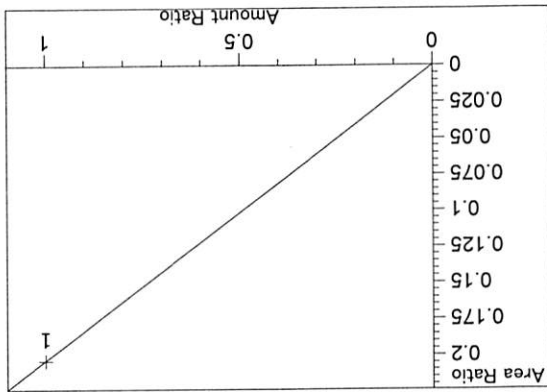

ethanol at exp. RT: 4.285
 FID2 B, Back Signal
 Correlation: 0.99992
 Residual Std. Dev.: 0.00532
 Formula: $Y = mx + b$
 m: 2.00945
 b: -1.01647e-2
 x: Amount Ratio
 Y: Area Ratio

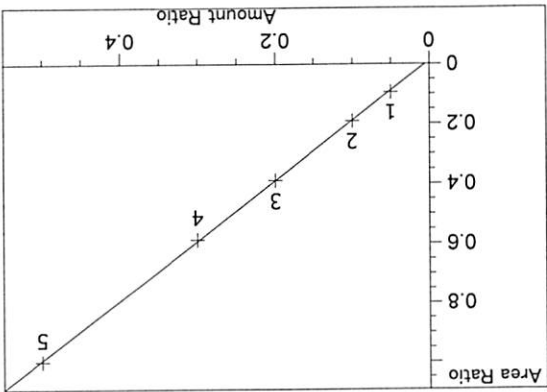


acetone at exp. RT: 4.308
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $Y = mx + b$
 m: 1.36147e-1
 b: 0.00000
 x: Amount Ratio
 Y: Area Ratio

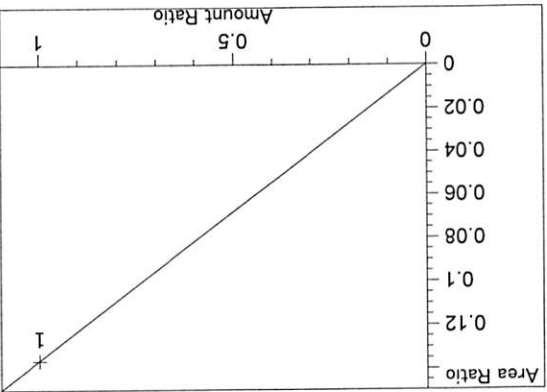


pk


n-propanol at exp. RT: 4.620
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $Y = mx + b$
 m: 1.00000
 b: 0.00000
 x: Amount Ratio
 Y: Area Ratio

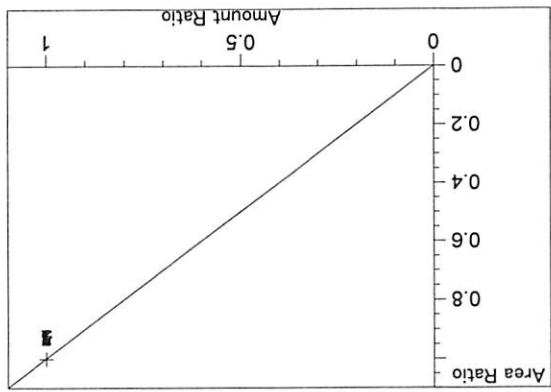


acetone at exp. RT: 4.661
 FID2 B, Back Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $Y = mx + b$
 m: $1.39199e-1$
 b: 0.00000
 x: Amount Ratio
 Y: Area Ratio

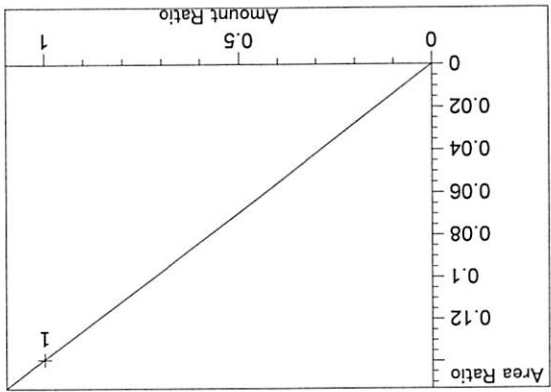

isopropyl alcohol at exp. RT: 4.969
 FID2 B, Back Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $Y = mx + b$
 m: $2.16208e-1$
 b: 0.00000
 x: Amount Ratio
 Y: Area Ratio

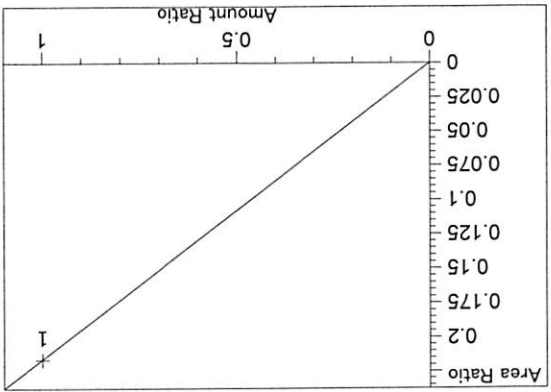

n-propanol at exp. RT: 7.550
 FID2 B, Back Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $Y = mx + b$
 m: 1.00000
 b: 0.00000
 x: Amount Ratio
 Y: Area Ratio

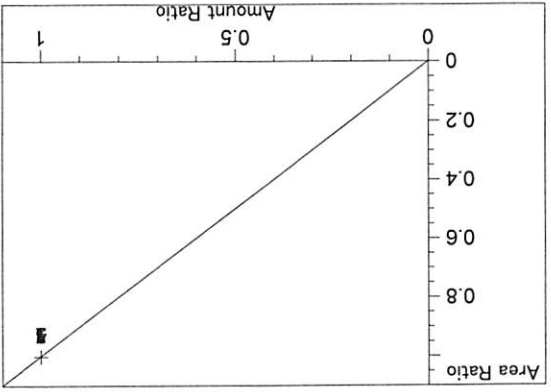


=====



I SP Forensic Services Blood Alcohol Report


Sample Name : 0.050 FN05211804
 Laboratory : Meridian
 Injection Date : Sep 18, 2020
 Method : ALCOHOL.M
 Acq. Instrument : CN1180014-CN11041167

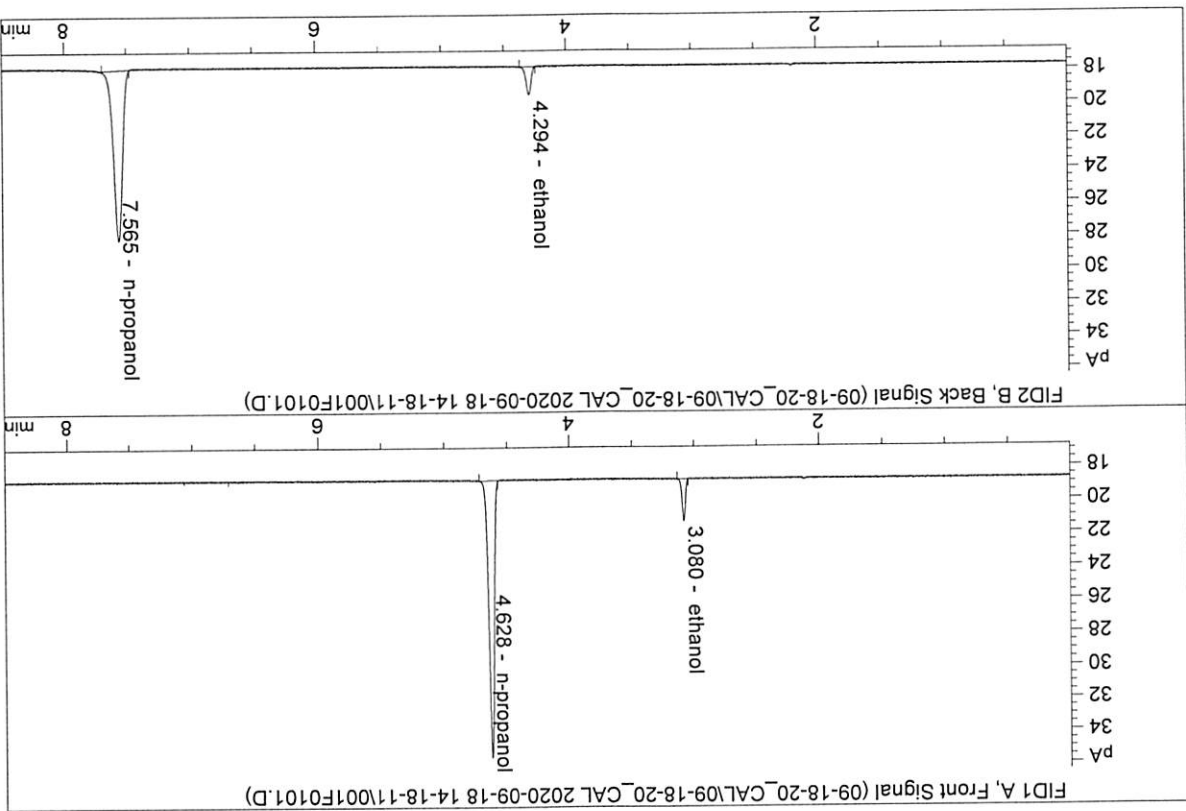

| # | Compound | Column | Area | Amount | Units |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol | Column 1: | 4.59217 | 0.0506 | g/100cc |
| 2. | Ethanol | Column 2: | 4.68252 | 0.0521 | g/100cc |
| 3. | n-Propanol | Column 1: | 47.73816 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 49.51909 | 1.0000 | g/100cc |

ISP Forensic Services Blood Alcohol Report


Sample Name : 0.100 FN02271802
 Laboratory : Meridian
 Injection Date : Sep 18, 2020
 Method : ALCOHOL.M
 Acq. Instrument : CN1180014-CN11041167

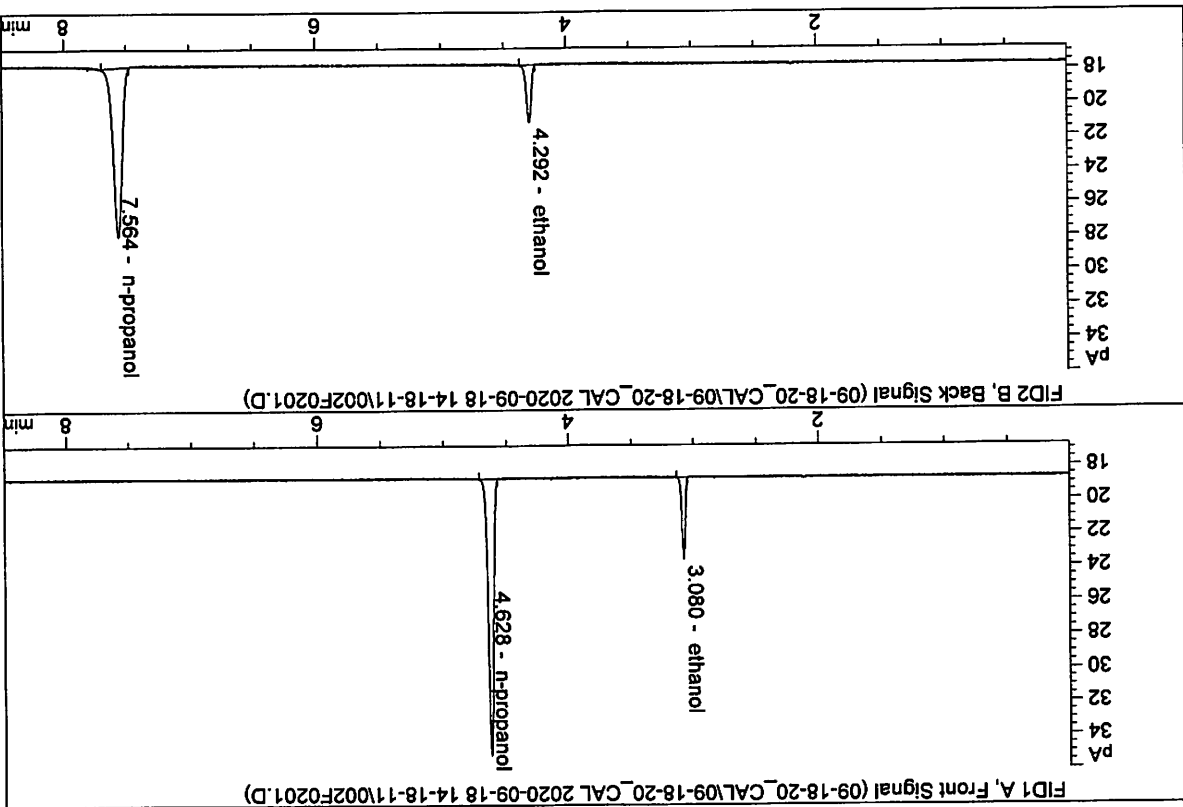

| # | Compound | Column | Area | Amount | Units |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol | Column 1: | 9.00449 | 0.1002 | g/100cc |
| 2. | Ethanol | Column 2: | 9.24722 | 0.1000 | g/100cc |
| 3. | n-Propanol | Column 1: | 46.90596 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 48.45788 | 1.0000 | g/100cc |

ISP Forensic Services Blood Alcohol Report


Sample Name : 0.200 FN06231704
 Laboratory : Meridian
 Injection Date : Sep 18, 2020
 Method : ALCOHOL.M
 Acq. Instrument : CN1180014-CN11041167

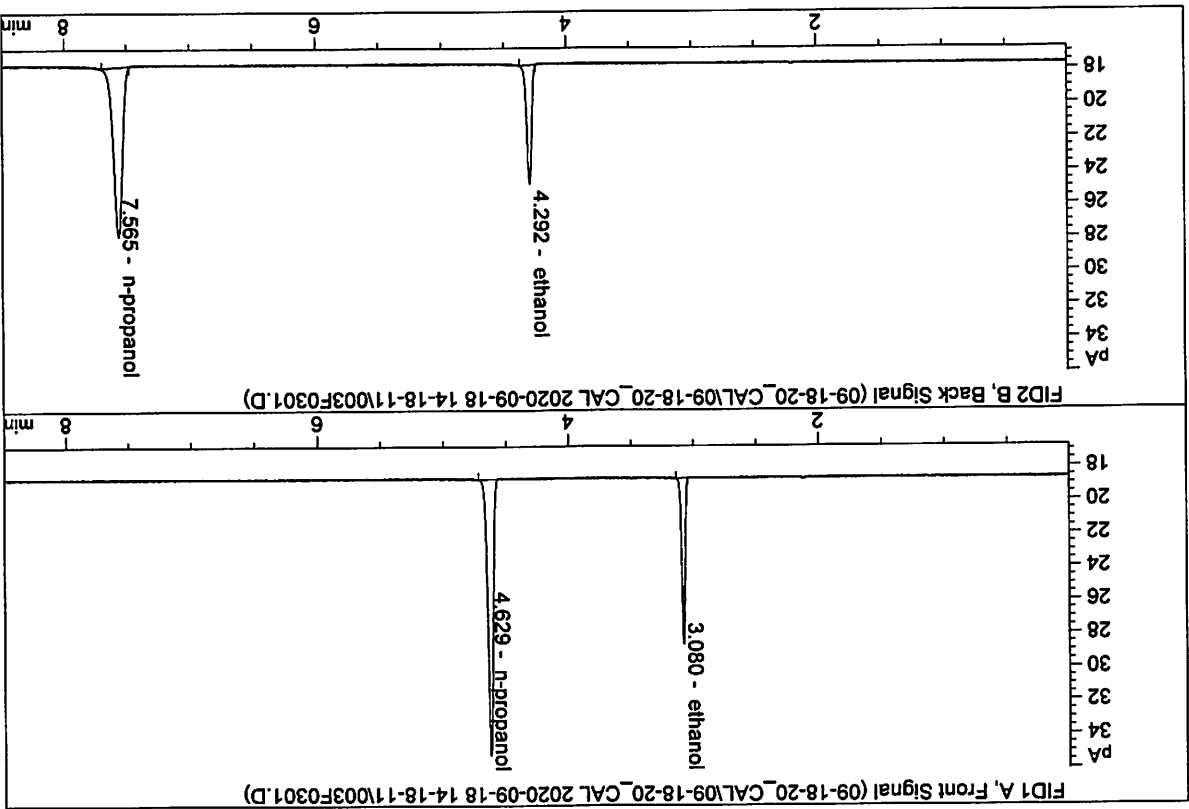

| # | Compound | Column | Area | Amount | Units |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol | Column 1: | 18.11074 | 0.2000 | g/100cc |
| 2. | Ethanol | Column 2: | 18.83116 | 0.1990 | g/100cc |
| 3. | n-Propanol | Column 1: | 47.03720 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 48.32198 | 1.0000 | g/100cc |

ISP Forensic Services Blood Alcohol Report


Sample Name : 0.300 FN07311804
 Laboratory : Meridian
 Injection Date : Sep 18, 2020
 Method : ALCOHOL.M
 Acq. Instrument : CN1180014-CN11041167

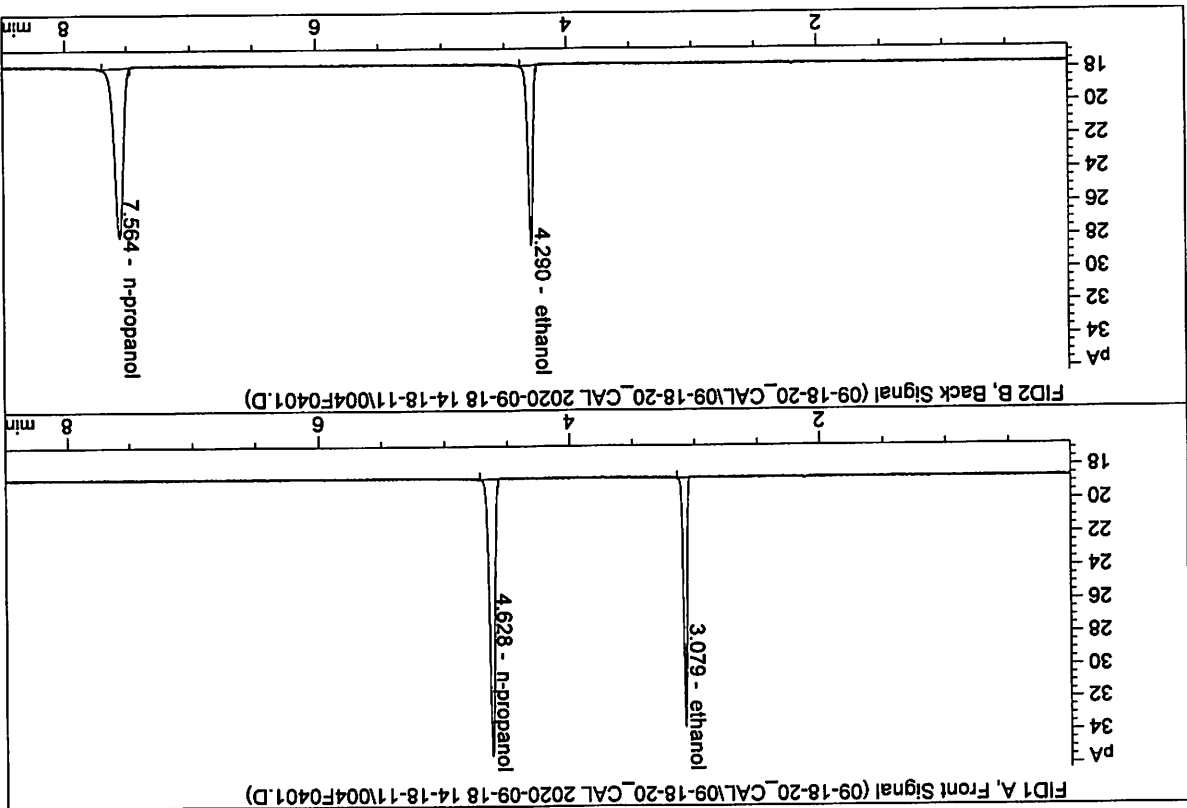

| # | Compound | Column | Area | Amount | Units |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol | Column 1: | 27.45135 | 0.2983 | g/100cc |
| 2. | Ethanol | Column 2: | 28.72548 | 0.2967 | g/100cc |
| 3. | n-Propanol | Column 1: | 47.72957 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 49.01604 | 1.0000 | g/100cc |

ISP Forensic Services Blood Alcohol Report


Sample Name : 0.500 FN08241801
 Laboratory : Meridian
 Injection Date : Sep 18, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN1180014-CN11041167

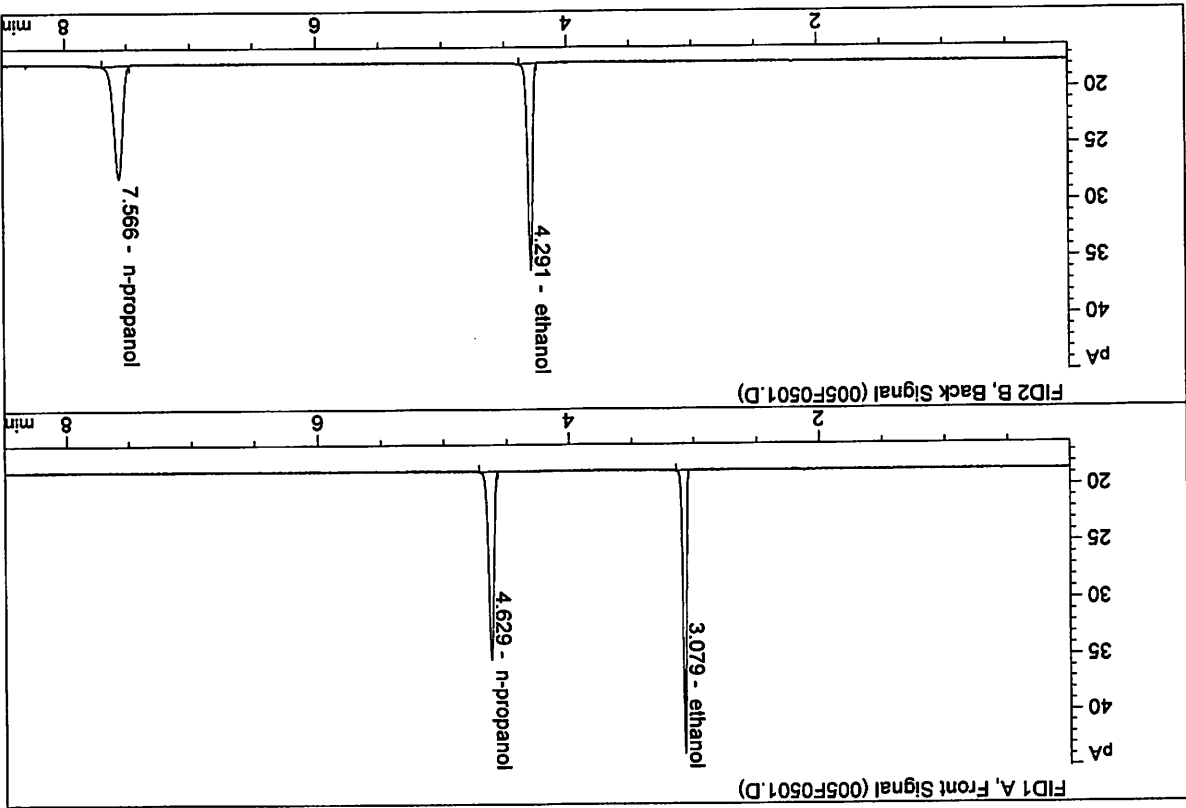

| # | Compound | Column | Area | Amount | Units |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol | Column 1: | 45.73181 | 0.5009 | g/100cc |
| 2. | Ethanol | Column 2: | 48.32216 | 0.5022 | g/100cc |
| 3. | n-Propanol | Column 1: | 47.28825 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 48.37467 | 1.0000 | g/100cc |

ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STANDARD BLANK
 Laboratory : Meridian
 Injection Date : Sep 18, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN1180014-CN11041167

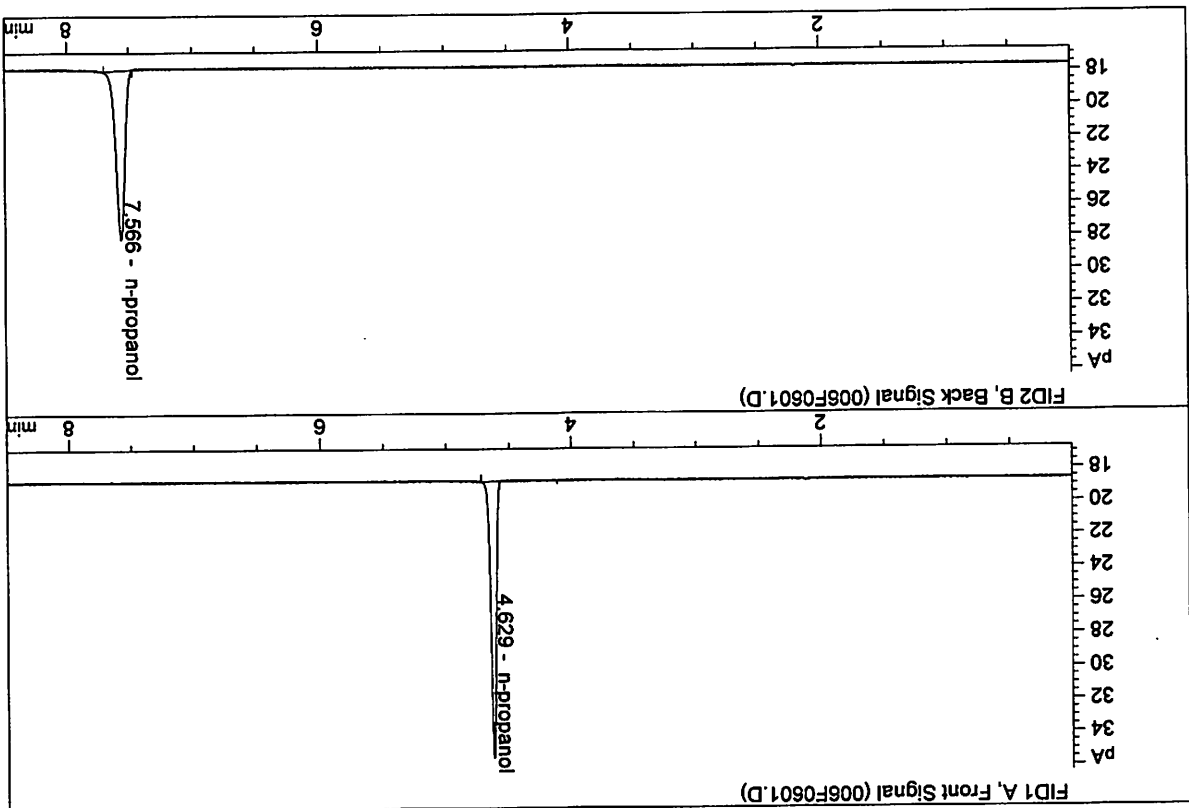

| # | Compound | Column | Area | Amount | Units |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol | Column 1: | 0.00000 | 0.0000 | g/100cc |
| 2. | Ethanol | Column 2: | 0.00000 | 0.0000 | g/100cc |
| 3. | n-Propanol | Column 1: | 47.83927 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 49.12637 | 1.0000 | g/100cc |

26

s a m p l e s u m m a r y

Sequence table: C:\Chem32\1\data\09-18-20\CAL\09-18-20\CAL 2020-09-18 14-18-11\09-18-20_CAL.S

Data directory path: C:\Chem32\1\data\09-18-20\CAL\09-18-20\CAL 2020-09-18 14-18-11\

Logbook: C:\Chem32\1\data\09-18-20\CAL\09-18-20\CAL 2020-09-18 14-18-11\09-18-20_CAL.LOG

Sequence start: 9/18/2020 2:32:48 PM

Sequence Operator: SYSTEM


Operator: SYSTEM

Method file name: C:\Chem32\1\data\09-18-20\CAL\09-18-20\CAL 2020-09-18 14-18-11\ALCOHOL.M

| Run Location Inj | # | Sample Name | Sample Amt | Multip.* | File name | Cal # | Cmp # |
|------------------|---|-------------------|------------|------------|-----------|-------|-------|
| 1 1 | 1 | 0.050 FN05211804 | 1.0000 | 001F0101.D | | 4 | * |
| 2 2 | 1 | 0.100 FN02271802 | 1.0000 | 002F0201.D | | 4 | * |
| 3 3 | 1 | 0.200 FN06231704 | 1.0000 | 003F0301.D | | 4 | * |
| 4 4 | 1 | 0.300 FN07311804 | 1.0000 | 004F0401.D | | 4 | * |
| 5 5 | 1 | 0.500 FN08241801 | 1.0000 | 005F0501.D | | 4 | * |
| 6 6 | 1 | INTERNAL STANDARD | 1.0000 | 006F0601.D | | 2 | |

ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STD BLK 1
 Laboratory : Meridian
 Injection Date : Sep 18, 2020
 Method : ALCOHOL.M
 Acq. Instrument : CN1180014-CN11041167

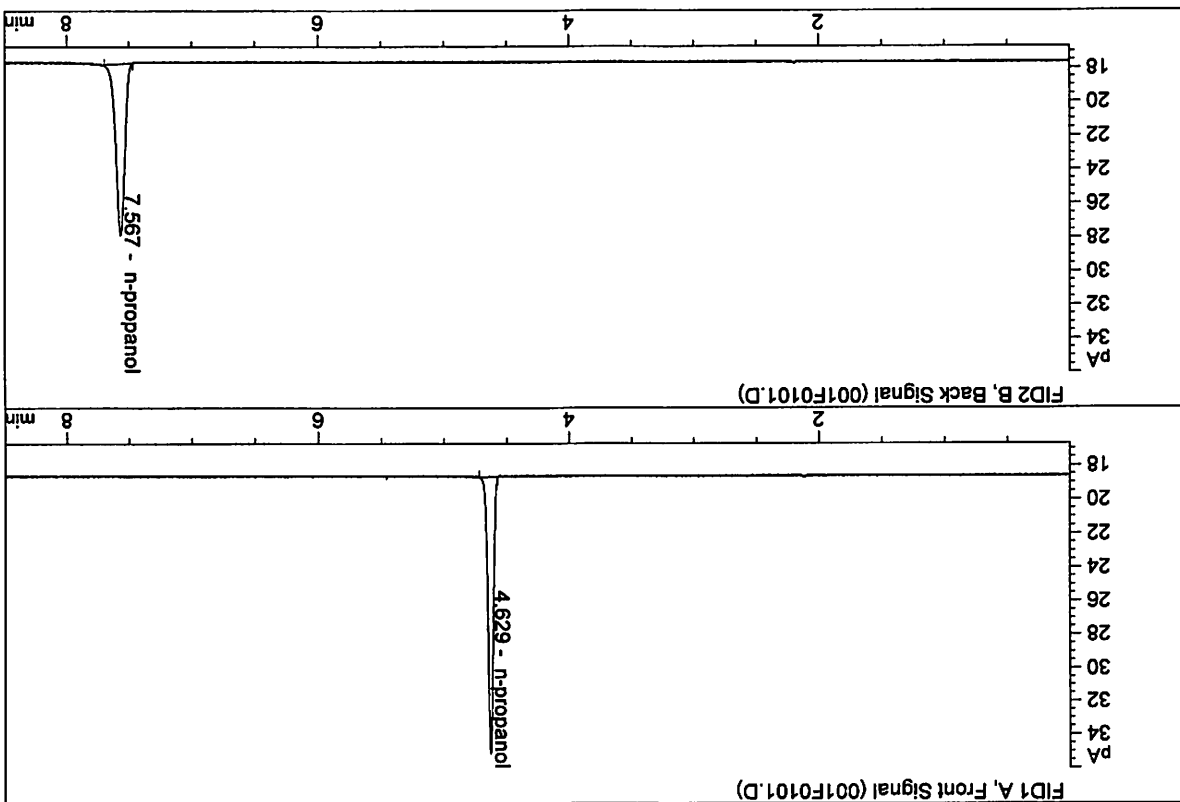


| # | Compound | Column | Area | Amount | Units |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol | Column 1: | 0.00000 | 0.0000 | g/100cc |
| 2. | Ethanol | Column 2: | 0.00000 | 0.0000 | g/100cc |
| 3. | n-Propanol | Column 1: | 46.92888 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 48.40623 | 1.0000 | g/100cc |

pc

ISP Forensic Services Blood Alcohol Report

Sample Name : MIX VOL FN07101701
 Laboratory : Meridian
 Injection Date : Sep 18, 2020
 Method : ALCOHOL.M
 Acq. Instrument : CN11180014-CN11041167

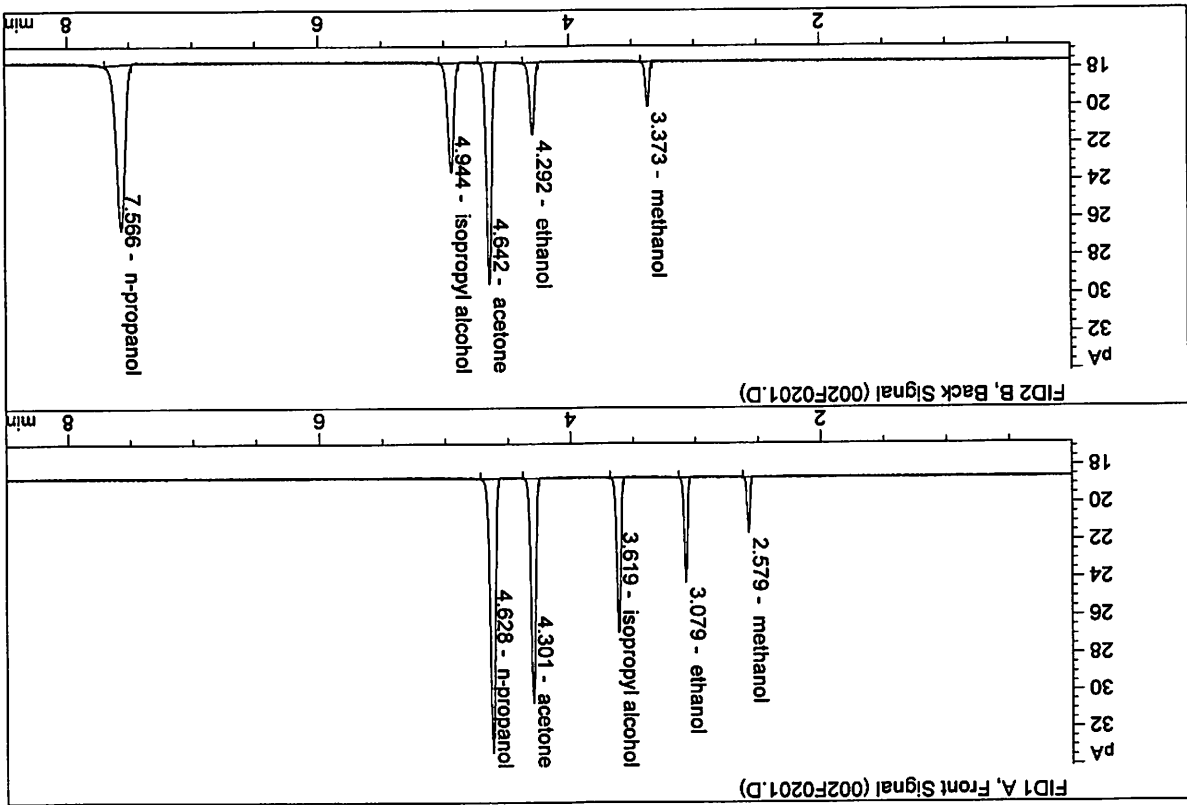

| # | Compound | Column | Area | Amount | Units |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol | Column 1: | 9.91866 | 0.1244 | g/100cc |
| 2. | Ethanol | Column 2: | 10.22028 | 0.1252 | g/100cc |
| 3. | n-Propanol | Column 1: | 41.53161 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 42.33088 | 1.0000 | g/100cc |

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC1-1 Analysis Date(s): 18 Sep 2020

| Sample Results | Column 1 FID A | Column 2 FID B | Column Precision | Mean Value | Sample A-B Difference | Over-all Mean |
|----------------|-------------------|-------------------|------------------|------------|--------------------------|---------------|
| (g/100cc) | 0.0730 | 0.0737 | 0.0007 | 0.0738 | 0.0005 | 0.0735 |
| | 0.0733 | 0.0743 | 0.0010 | 0.0738 | | |

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument information is stored centrally.

Refer to Instrument Method: Alcohol.m

Reporting of Results
Uncertainty of Measurement (UM%): 5.00%

| Overall Mean (g/100cc) | Low | High | 5% of Mean |
|------------------------|-------|-------|------------|
| 0.073 | 0.069 | 0.077 | 0.004 |

Reported Result


0.073

Calibration and control data are stored centrally.



ISP Forensic Services Blood Alcohol Report


Sample Name : Q1-1-A
 Laboratory : Meridian
 Injection Date : Sep 18, 2020
 Method : ALCOHOL.M
 Instrument: CN1180014-CN11041167

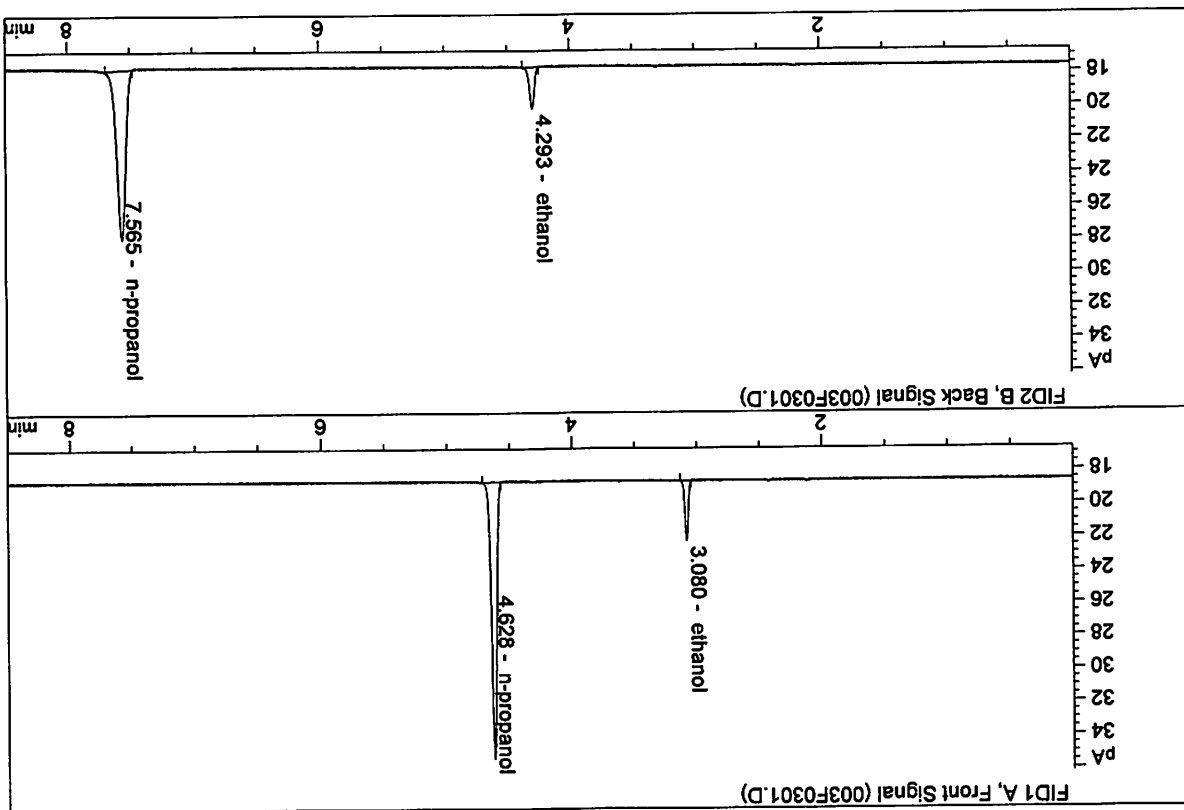

| # | Compound | Column | Area | Amount | Units |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol | Column 1: | 6.62145 | 0.0730 | g/100cc |
| 2. | Ethanol | Column 2: | 6.70895 | 0.0737 | g/100cc |
| 3. | n-Propanol | Column 1: | 47.50263 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 48.63763 | 1.0000 | g/100cc |

ISP Forensic Services Blood Alcohol Report

Sample Name : Q1-1-B
 Laboratory : Meridian
 Injection Date : Sep 18, 2020
 Method : ALCOHOL.M
 Acq. Instrument : CN1180014-CN11041167

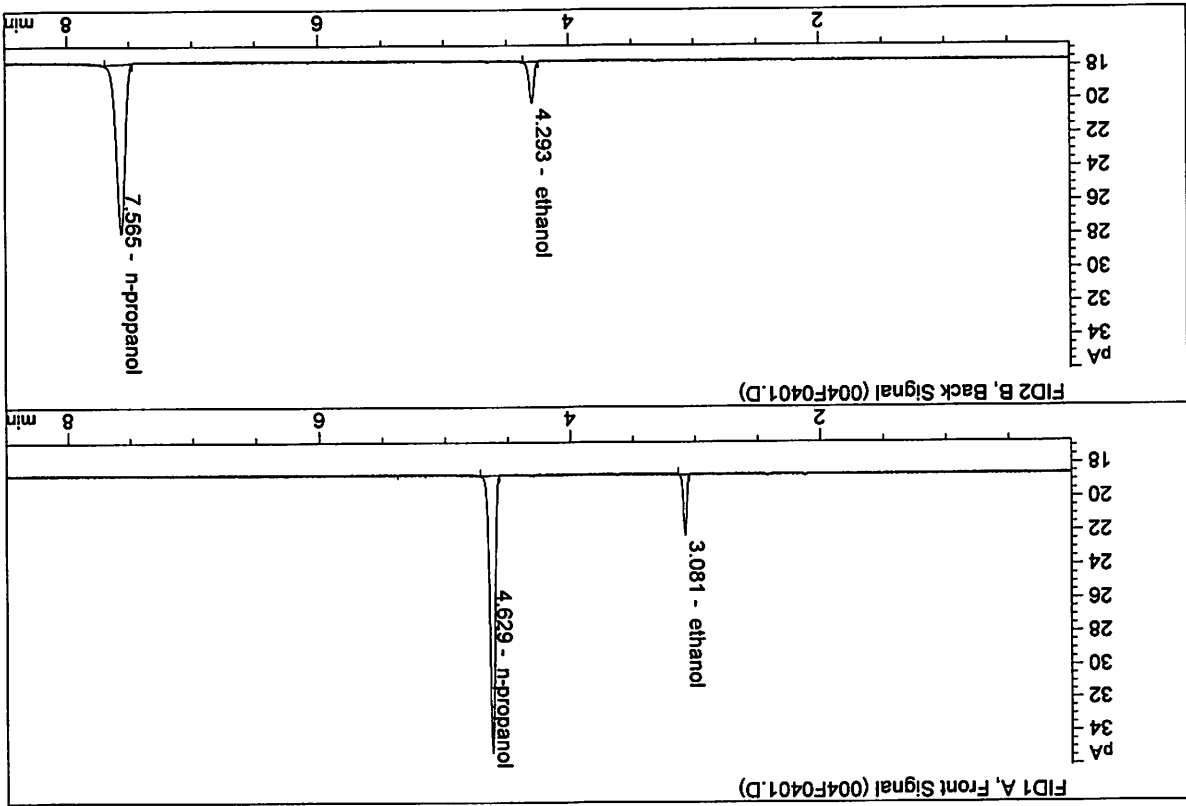

| # | Compound | Column | Area | Amount | Units |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol | Column 1: | 6.59871 | 0.0733 | g/100cc |
| 2. | Ethanol | Column 2: | 6.72393 | 0.0743 | g/100cc |
| 3. | n-Propanol | Column 1: | 47.14786 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 48.33992 | 1.0000 | g/100cc |

6

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: 08 FN04171701 Analysis Date(s): 18 Sep 2020

| | Column 1 FID A | Column 2 FID B | Column Precision | Mean Value | Sample A-B Difference | Over-all Mean |
|----------------|-------------------|-------------------|------------------|------------|--------------------------|---------------|
| Sample Results | 0.0794 | 0.0800 | 0.0006 | 0.0797 | 0.0007 | 0.0800 |
| (g/100cc) | 0.0800 | 0.0809 | 0.0009 | 0.0804 | | |

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Refer to Instrument Method: Alcohol.m

Reporting of Results

| Overall Mean (g/100cc) | Low | High | 5% of Mean |
|------------------------|-------|-------|------------|
| 0.080 | 0.076 | 0.084 | 0.004 |

Uncertainty of Measurement (UM%): 5.00%

Reported Result


0.080

Calibration and control data are stored centrally.



ISP Forensic Services Blood Alcohol Report

Sample Name : 0.08 FN04171701-A
 Laboratory : Meridian
 Injection Date : Sep 18, 2020
 Method : ALCOHOL.M
 Acq. Instrument : CN1180014-CN11041167

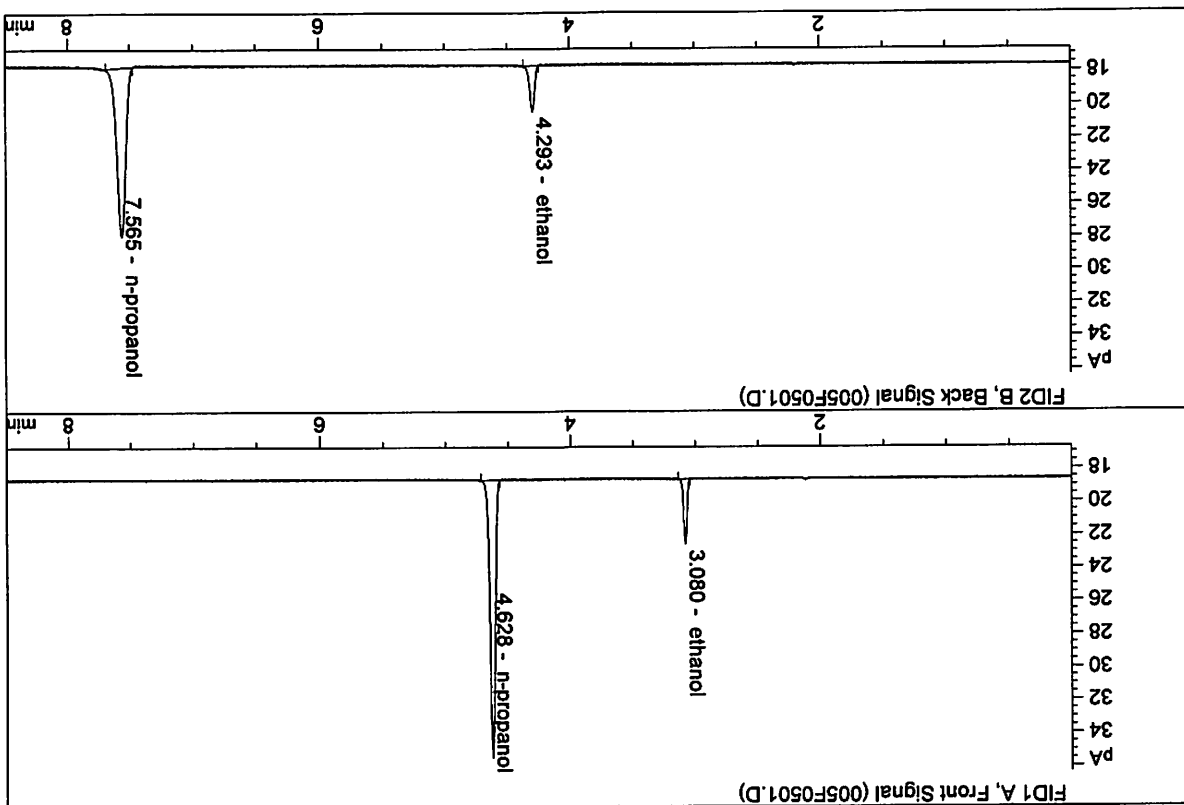


| # | Compound | Column | Area | Amount | Units |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol | Column 1: | 7.26391 | 0.0794 | g/100cc |
| 2. | Ethanol | Column 2: | 7.38075 | 0.0800 | g/100cc |
| 3. | n-Propanol | Column 1: | 47.84095 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 49.00060 | 1.0000 | g/100cc |

✓

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.08 FN04171701-B
 Laboratory : Meridian
 Injection Date : Sep 18, 2020
 Method : ALCOHOL.M
 Acq. Instrument : CN1180014-CN11041167

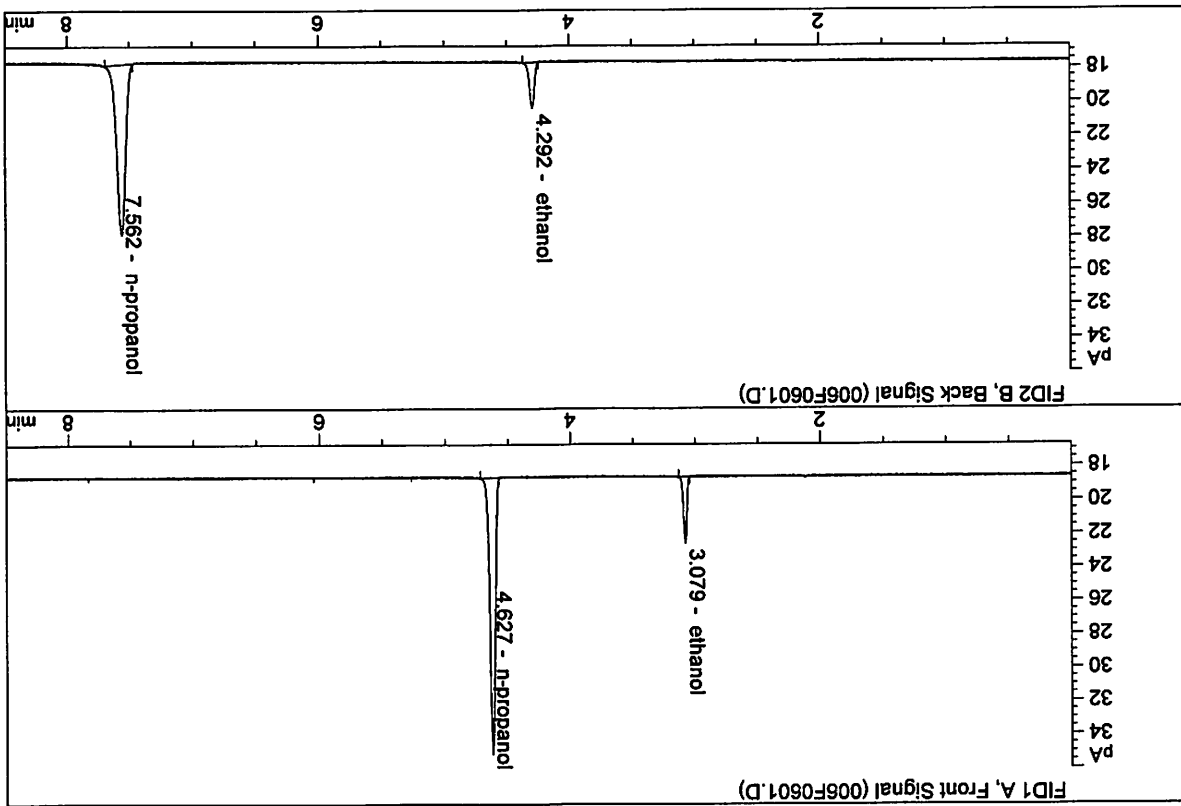

| # | Compound | Column | Area | Amount | Units |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol | Column 1: | 7.19459 | 0.0800 | g/100cc |
| 2. | Ethanol | Column 2: | 7.33517 | 0.0809 | g/100cc |
| 3. | n-Propanol | Column 1: | 47.03626 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 48.10363 | 1.0000 | g/100cc |

10

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC2-1 Analysis Date(s): 18 Sep 2020

| | Column 1 FID A | Column 2 FID B | Column Precision | Mean Value | Sample A-B Difference | Over-all Mean |
|----------------|-------------------|-------------------|------------------|------------|--------------------------|---------------|
| Sample Results | 0.1995 | 0.1987 | 0.0008 | 0.1991 | 0.0013 | 0.1984 |
| (g/100cc) | 0.1978 | 0.1978 | 0.0000 | 0.1978 | | |

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Refer to Instrument Method: Alcohol.m

Reporting of Results

| Overall Mean (g/100cc) | Low | High | 5% of Mean |
|------------------------|-------|-------|------------|
| 0.198 | 0.188 | 0.208 | 0.010 |

Uncertainty of Measurement (UM%): 5.00%

Reported Result


0.198

Calibration and control data are stored centrally.



ISP Forensic Services Blood Alcohol Report


Sample Name : QC2-1-A
 Laboratory : Meridian
 Injection Date : Sep 18, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

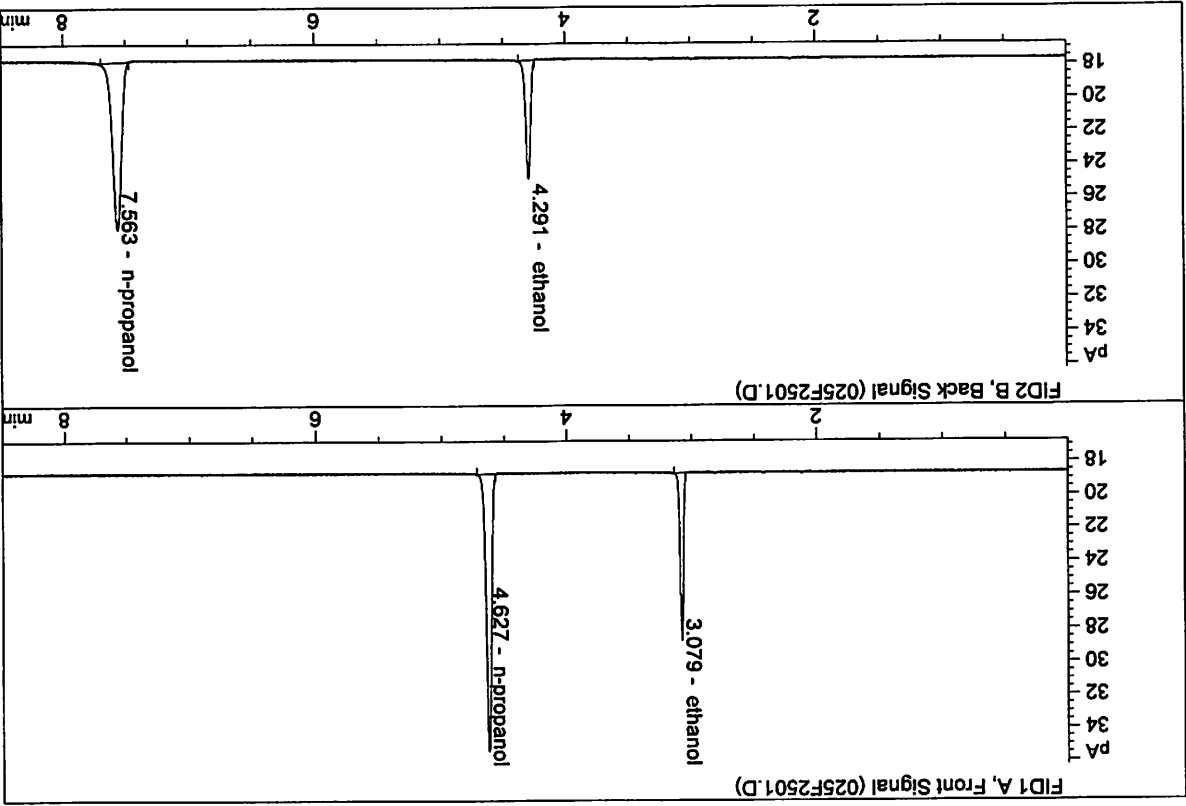

| # | Compound | Column | Area | Amount | Units |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol | Column 1: | 18.31867 | 0.1995 | g/100cc |
| 2. | Ethanol | Column 2: | 18.94781 | 0.1987 | g/100cc |
| 3. | n-Propanol | Column 1: | 47.70006 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 48.69275 | 1.0000 | g/100cc |

ISP Forensic Services Blood Alcohol Report

Sample Name : QC2-1-B
 Laboratory : Meridian
 Injection Date : Sep 18, 2020
 Method : ALCOHOL.M
 Acq. Instrument : CN11180014-CN11041167

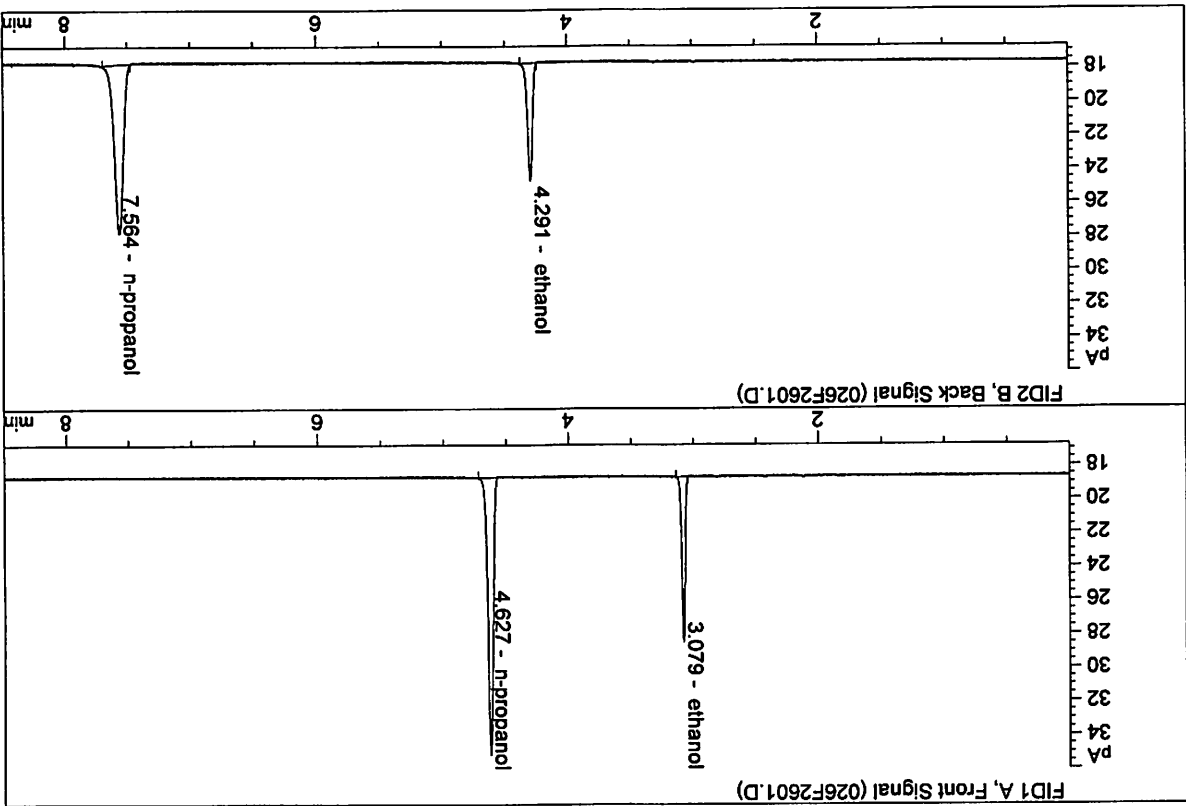

| # | Compound | Column | Area | Amount | Units |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol | Column 1: | 17.90640 | 0.1978 | g/100cc |
| 2. | Ethanol | Column 2: | 18.59531 | 0.1978 | g/100cc |
| 3. | n-Propanol | Column 1: | 47.03071 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 48.00474 | 1.0000 | g/100cc |

Calibration and control data are stored centrally.


| | | | | | | |
|--|----------|------------------|------------|-----------------------|---------------|-----------|
| Reporting of Results Uncertainty of Measurement (UM%): 5.00% | | | | | | |
| Overall Mean (g/100cc) | | | Low | High | 5% of Mean | |
| 0.074 | | | 0.070 | 0.078 | 0.004 | |
| Reported Result | | | 0.074 | | | |
| Analysis Method Refer to Blood Alcohol Method #1 | | | | | | |
| Instrument Information Refer to Instrument Method: Alcohol.m Instrument information is stored centrally. | | | | | | |
| Column 1 | Column 2 | Column Precision | Mean Value | Sample A-B Difference | Over-all Mean | |
| FID A | FID B | | | | | |
| 0.0740 | 0.0751 | 0.0011 | 0.0745 | 0.0005 | 0.0747 | |
| 0.0743 | 0.0757 | 0.0014 | 0.0750 | | | (g/100cc) |

Laboratory No.: QC1-2 Analysis Date(s): 19 Sep 2020

VOLATILES DETERMINATION CASEFILE WORKSHEET

ISP Forensic Services Blood Alcohol Report

Sample Name : Q1-2-A
 Laboratory : Meridian
 Injection Date : Sep 19, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN1180014-CN11041167

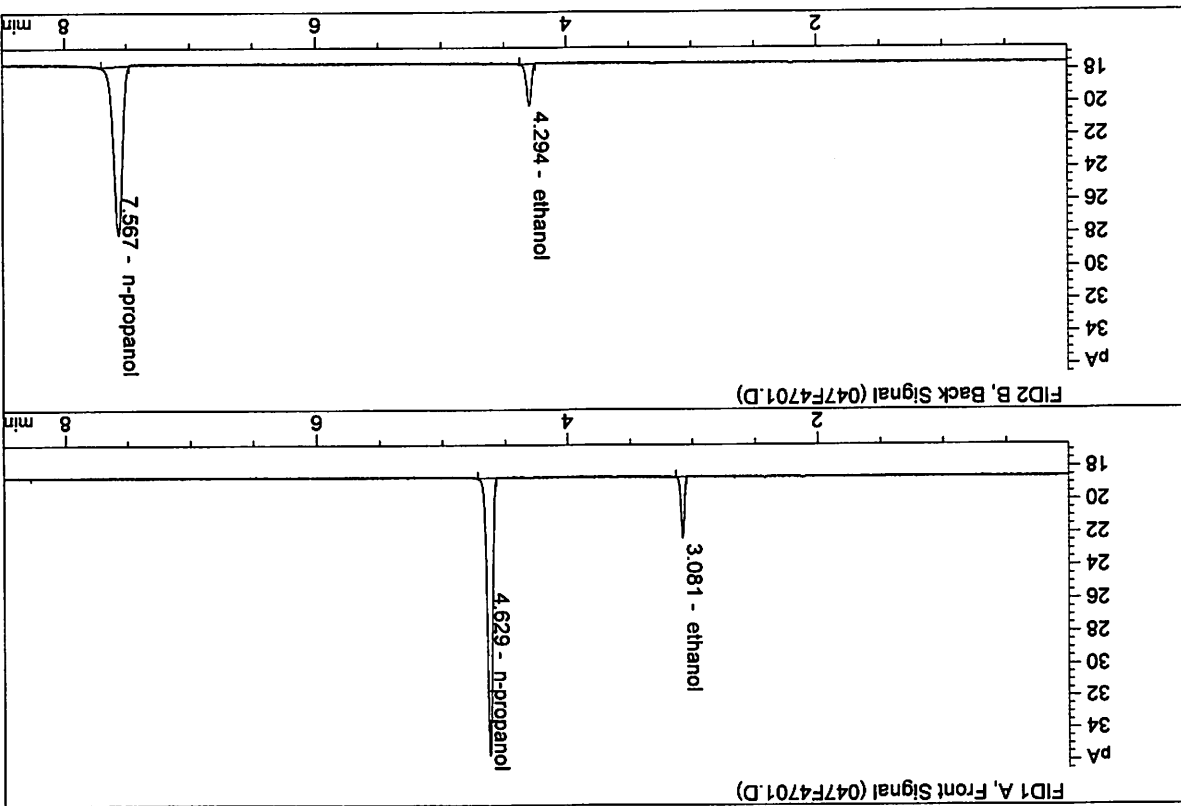


| # | Compound | Column | Area | Amount | Units |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol | Column 1: | 6.86763 | 0.0740 | g/100cc |
| 2. | Ethanol | Column 2: | 6.99981 | 0.0751 | g/100cc |
| 3. | n-Propanol | Column 1: | 48.55942 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 49.71533 | 1.0000 | g/100cc |

✓


ISP Forensic Services Blood Alcohol Report

Sample Name : Q1-2-B
 Laboratory : Meridian
 Injection Date : Sep 19, 2020
 Method : ALCOHOL.M
 Instrument: CN1180014-CN11041167

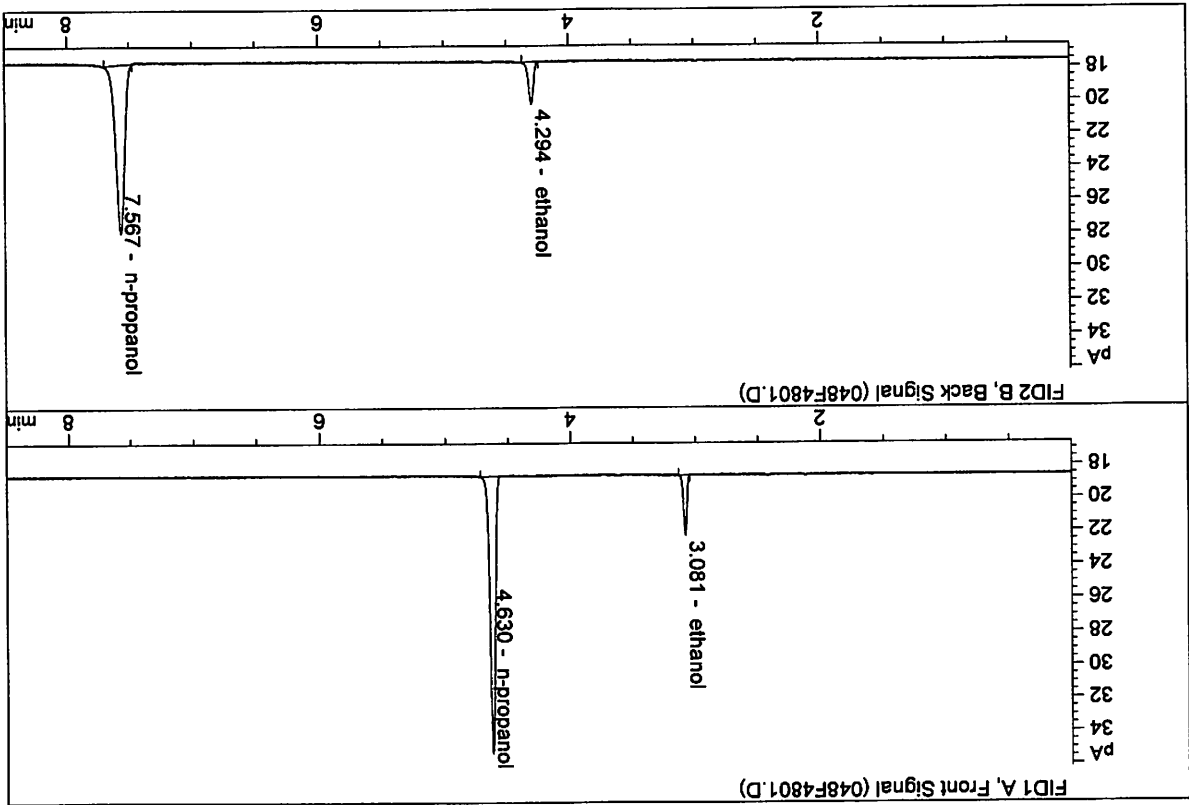

| # | Compound | Column | Area | Amount | Units |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol | Column 1: | 6.75266 | 0.0743 | g/100cc |
| 2. | Ethanol | Column 2: | 6.90275 | 0.0757 | g/100cc |
| 3. | n-Propanol | Column 1: | 47.58894 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 48.61000 | 1.0000 | g/100cc |

Sample Name : INTERNAL STD BLK
 Laboratory : Meridian
 Injection Date : Sep 19, 2020
 Method : ALCOHOL.M
 Acq. Instrument : CN1180014-CN11041167

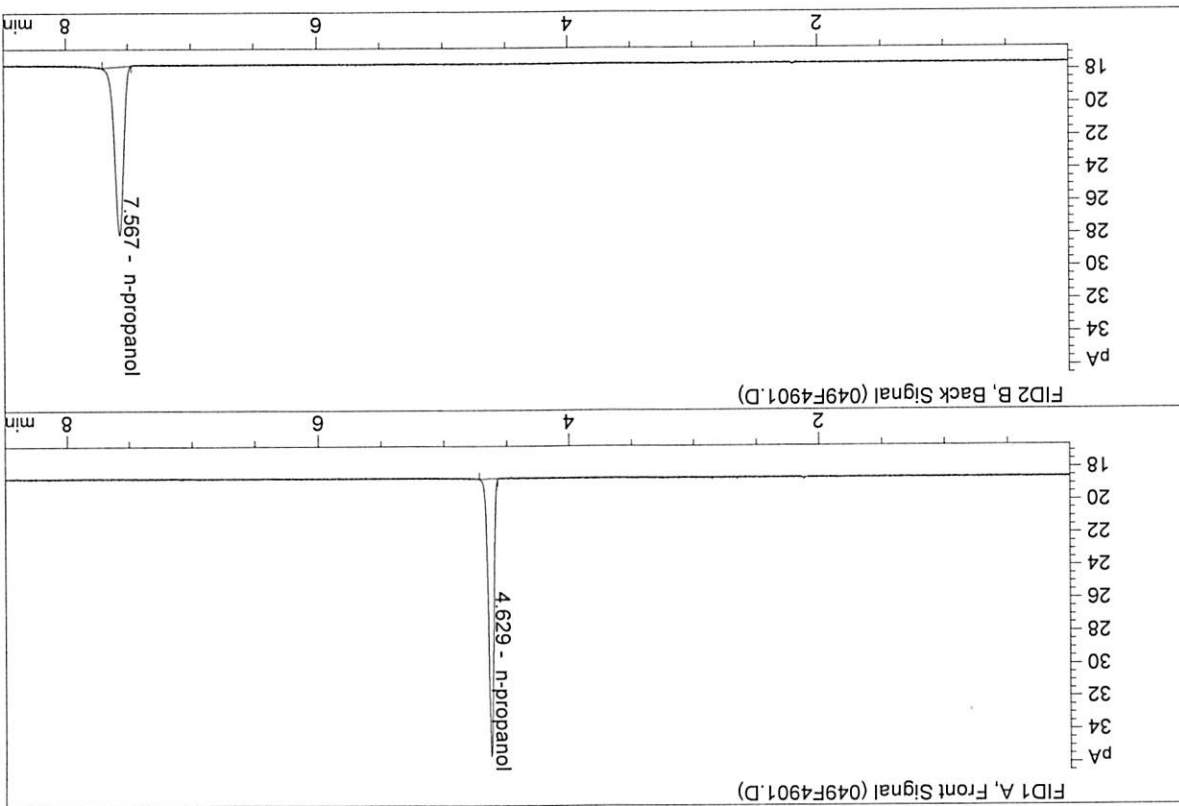

| # | Compound | Column | Area | Amount | Units |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol | Column 1: | 0.00000 | 0.0000 | g/100cc |
| 2. | Ethanol | Column 2: | 0.00000 | 0.0000 | g/100cc |
| 3. | n-Propanol | Column 1: | 48.22735 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 49.57272 | 1.0000 | g/100cc |

S a m p l e s u m m a r y

Sequence table: C:\chem32\1\Data\09-18-20\SAMPLES 2020-09-18 15-45-41\09-18-20\SAMPLES.S
 Data directory path: C:\chem32\1\Data\09-18-20\SAMPLES 2020-09-18 15-45-41\09-18-20\SAMPLES.LOG
 Logbook: C:\chem32\1\Data\09-18-20\SAMPLES 2020-09-18 15-45-41\09-18-20\SAMPLES.S
 Sequence start: 9/18/2020 4:00:27 PM
 Sequence Operator: SYSTEM
 Operator: SYSTEM
 Method file name: C:\chem32\1\Data\09-18-20\SAMPLES 2020-09-18 15-45-41\ALCOHOL.M

| Run Location Inj # | Sample Name | Sample Amt [g/100cc] | Multip. * | File name | Cal # | Cmp # |
|--------------------|-------------|----------------------|-----------|-----------|-------|-------|
|--------------------|-------------|----------------------|-----------|-----------|-------|-------|

| | | | | | | |
|----|----|--------------------|---|--------|------------|----|
| 1 | 1 | INTERNAL STD BLK | - | 1.0000 | 001F0101.D | 2 |
| 2 | 2 | MIX VOL FN071017 | - | 1.0000 | 002F0201.D | 10 |
| 3 | 3 | QC1-1-A | - | 1.0000 | 003F0301.D | 4 |
| 4 | 4 | QC1-1-B | - | 1.0000 | 004F0401.D | 4 |
| 5 | 5 | 1 0.08 FN04171701- | - | 1.0000 | 005F0501.D | 4 |
| 6 | 6 | 1 0.08 FN04171701- | - | 1.0000 | 006F0601.D | 4 |
| 7 | 7 | 1 M2020-3449-2-A | - | 1.0000 | 007F0701.D | 2 |
| 8 | 8 | 1 M2020-3449-2-B | - | 1.0000 | 008F0801.D | 2 |
| 9 | 9 | 1 M2020-3510-1-A | - | 1.0000 | 009F0901.D | 4 |
| 10 | 10 | 1 M2020-3510-1-B | - | 1.0000 | 010F1001.D | 4 |
| 11 | 11 | 1 M2020-3510-2-A | - | 1.0000 | 011F1101.D | 3 |
| 12 | 12 | 1 M2020-3510-2-B | - | 1.0000 | 012F1201.D | 3 |
| 13 | 13 | 1 M2020-3510-3-A | - | 1.0000 | 013F1301.D | 4 |
| 14 | 14 | 1 M2020-3510-3-B | - | 1.0000 | 014F1401.D | 4 |
| 15 | 15 | 1 M2020-3510-4-A | - | 1.0000 | 015F1501.D | 4 |
| 16 | 16 | 1 M2020-3510-4-B | - | 1.0000 | 016F1601.D | 4 |
| 17 | 17 | 1 M2020-3538-1-A | - | 1.0000 | 017F1701.D | 4 |
| 18 | 18 | 1 M2020-3538-1-B | - | 1.0000 | 018F1801.D | 4 |
| 19 | 19 | 1 M2020-3539-1-A | - | 1.0000 | 019F1901.D | 4 |
| 20 | 20 | 1 M2020-3539-1-B | - | 1.0000 | 020F2001.D | 4 |
| 21 | 21 | 1 M2020-3584-1-A | - | 1.0000 | 021F2101.D | 2 |
| 22 | 22 | 1 M2020-3584-1-B | - | 1.0000 | 022F2201.D | 2 |
| 23 | 23 | 1 M2020-3585-1-A | - | 1.0000 | 023F2301.D | 2 |
| 24 | 24 | 1 M2020-3585-1-B | - | 1.0000 | 024F2401.D | 2 |
| 25 | 25 | 1 QC2-1-A | - | 1.0000 | 025F2501.D | 4 |
| 26 | 26 | 1 QC2-1-B | - | 1.0000 | 026F2601.D | 4 |
| 27 | 27 | 1 M2020-3598-1-A | - | 1.0000 | 027F2701.D | 4 |
| 28 | 28 | 1 M2020-3598-1-B | - | 1.0000 | 028F2801.D | 4 |
| 29 | 29 | 1 M2020-3632-1-A | - | 1.0000 | 029F2901.D | 4 |
| 30 | 30 | 1 M2020-3632-1-B | - | 1.0000 | 030F3001.D | 4 |
| 31 | 31 | 1 M2020-3642-1-A | - | 1.0000 | 031F3101.D | 4 |
| 32 | 32 | 1 M2020-3642-1-B | - | 1.0000 | 032F3201.D | 4 |
| 33 | 33 | 1 M2020-3660-1-A | - | 1.0000 | 033F3301.D | 4 |
| 34 | 34 | 1 M2020-3660-1-B | - | 1.0000 | 034F3401.D | 4 |
| 35 | 35 | 1 M2020-3661-1-A | - | 1.0000 | 035F3501.D | 2 |
| 36 | 36 | 1 M2020-3661-1-B | - | 1.0000 | 036F3601.D | 2 |
| 37 | 37 | 1 M2020-3668-1-A | - | 1.0000 | 037F3701.D | 4 |
| 38 | 38 | 1 M2020-3668-1-B | - | 1.0000 | 038F3801.D | 4 |
| 39 | 39 | 1 M2020-3688-1-A | - | 1.0000 | 039F3901.D | 4 |
| 40 | 40 | 1 M2020-3688-1-B | - | 1.0000 | 040F4001.D | 4 |
| 41 | 41 | 1 M2020-3689-1-A | - | 1.0000 | 041F4101.D | 4 |
| 42 | 42 | 1 M2020-3689-1-B | - | 1.0000 | 042F4201.D | 4 |
| 43 | 43 | 1 M2020-3701-1-A | - | 1.0000 | 043F4301.D | 4 |

QC 1-A 35

36

| Run Location Inj | Sample Name | Sample Amt | Multip.* | File name | Cal # | Cmp # |
|------------------|--------------------|------------|------------|-----------|-------|-------|
| 44 44 | 1 M2020-3701-1-B | 1.0000 | 044F4401.D | | 4 | |
| 45 45 | 1 P2020-2169-2-A | 1.0000 | 045F4501.D | | 2 | |
| 46 46 | 1 P2020-2169-2-B | 1.0000 | 046F4601.D | | 2 | |
| 47 47 | 1 Q01-2-A | 1.0000 | 047F4701.D | | 4 | |
| 48 48 | 1 Q01-2-B | 1.0000 | 048F4801.D | | 4 | |
| 49 49 | 1 INTERNAL STD BLK | 1.0000 | 049F4901.D | | 2 | |

Method file name: C:\chem32\1\Data\09-18-20_SAMPLES\09-18-20_SAMPLES 2020-09-18 15-45-41 \SHUTDOWN.M

| Run Location Inj | Sample Name | Sample Amt | Multip.* | File name | Cal # | Cmp # |
|------------------|-------------|------------|----------|------------|-------|-------|
| 50 50 | 1 EMPTY | - | 1.0000 | 050F5001.D | 0 | |

JK