
























Worklist: 1305

central data reviewed by B. Wylie on 10-6-16

10/5/2016



<u>LAB_CASE</u>	<u>ITEM</u>	<u>TASK_ID</u>	<u>DESCRIPTION</u>	
M2016-1637	1	55269	3.6.1 Blood base neutral confirr	
M2016-1674	1	55397	3.6.1 Blood base neutral confirr	
M2016-1779	1	55621	3.6.1 Blood base neutral confirr	
M2016-1784	1	55633	3.6.1 Blood base neutral confirr	
M2016-1863	1	55986	3.6.1 Blood base neutral confirr	
M2016-1904	1	56114	3.6.1 Blood base neutral confirr	
M2016-2037	1	56619	3.6.1 Blood base neutral confirr	
M2016-2070	2	56912	3.6.1 Blood base neutral confirr	
M2016-2204	2	57779	3.6.1 Blood base neutral confirr	
M2016-2863	2	60907	3.6.1 Blood base neutral confirr	
P2016-1139	1	56253	3.6.1 Blood base neutral confirr	
P2016-1174	1	56511	3.6.1 Blood base neutral confirr	
P2016-1184	1	56628	3.6.1 Blood base neutral confirr	
P2016-1191	1	56672	3.6.1 Blood base neutral confirr	
P2016-1205	2	56797	3.6.1 Blood base neutral confirr	
P2016-1206	1	56807	3.6.1 Blood base neutral confirr	
P2016-1209	1	56889	3.6.1 Blood base neutral confirr	
P2016-1210	1	56892	3.6.1 Blood base neutral confirr	
P2016-1211	1	56906	3.6.1 Blood base neutral confirr	
P2016-1212	1	56909	3.6.1 Blood base neutral confirr	
P2016-1214	1	56918	3.6.1 Blood base neutral confirr	
P2016-1301	1	57507	3.6.1 Blood base neutral confirr	
P2016-1327	1	57772	3.6.1 Blood base neutral confirr	

Worklist: 1305

<u>LAB CASE</u>	<u>ITEM</u>	<u>TASK ID</u>	<u>DESCRIPTION</u>
P2016-1359	1	58091	3.6.1 Blood base neutral confirr
P2016-1582	1	59681	3.6.1 Blood base neutral confirr



reviewed 10/19/16

Sequence Verified
JM 10/5/16

simulate_sequence.log
Simulate Run Sequence Wed Oct 05 10:56:12 2016

Instrument Name: Major Mass Spec
Sequence File: C:\Users\ISPuser\Desktop\Sequences\CS-BNSB080516.sequence.xml
Comment: MassHunter sequence
Operator: ISP\datastor
Data Path: D:\DATA\TM\2016\10052016\
Method Path: C:\Users\datastor\Desktop\OP Methods\

Line	Type	Vials	DataFile	Sample Name
Acquisition Method: BNSB120510.M				
1)	Sample	✓ 100	Prerun Solvent Blank	Pre-run Solvent Blank
2)	Sample	✓ 1	Negative Control-BN	Negative Control -
...	1013			
3)	Sample	✓ 2	Spiked Positive Control-BN	Positive Control
4)	Sample	✓ 99	prbLK2	Solvent Blank
Acquisition Method: GBT092509-Delta EMV.M				
5)	Sample	✓ 100	Prerun Solvent Blankr	Pre-run Solvent Blank
6)	Sample	✓ 1	Negative Control-BNr	Negative Control -
...	1013			
7)	Sample	✓ 2	Spiked Positive Control-BNr	Positive Control
8)	Sample	✓ 99	prbLK2r	Solvent Blank
Acquisition Method: BNSB120510.M				
9)	Sample	100	M2016-1637-1-BNBLK	Lab No.: M2016-1637-1
10)	Sample	✓ 3	M2016-1637-1-BN	Lab No.: M2016-1637-1
Acquisition Method: GBT092509-Delta EMV.M				
11)	Sample	✓ 3	M2016-1637-1-BNr	Lab No.: M2016-1637-1
Acquisition Method: BNSB120510.M				
12)	Sample	100	M2016-1674-1-BNBLK	Lab No.: M2016-1674-1
13)	Sample	✓ 4	M2016-1674-1-BN	Lab No.: M2016-1674-1
Acquisition Method: GBT092509-Delta EMV.M				
14)	Sample	✓ 4	M2016-1674-1-BNr	Lab No.: M2016-1674-1
Acquisition Method: BNSB120510.M				
15)	Sample	100	M2016-1779-1-BNBLK	Lab No.: M2016-1779-1
16)	Sample	✓ 5	M2016-1779-1-BN	Lab No.: M2016-1779-1
Acquisition Method: GBT092509-Delta EMV.M				
17)	Sample	✓ 5	M2016-1779-1-BNr	Lab No.: M2016-1779-1
Acquisition Method: BNSB120510.M				
18)	Sample	100	M2016-1784-1-BNBLK	Lab No.: M2016-1784-1
19)	Sample	✓ 6	M2016-1784-1-BN	Lab No.: M2016-1784-1
Acquisition Method: GBT092509-Delta EMV.M				
20)	Sample	✓ 6	M2016-1784-1-BNr	Lab No.: M2016-1784-1
Acquisition Method: BNSB120510.M				
21)	Sample	100	M2016-1863-1-BNBLK	Lab No.: M2016-1863-1
22)	Sample	✓ 7	M2016-1863-1-BN	Lab No.: M2016-1863-1
Acquisition Method: GBT092509-Delta EMV.M				
23)	Sample	✓ 7	M2016-1863-1-BNr	Lab No.: M2016-1863-1
Acquisition Method: BNSB120510.M				
24)	Sample	100	M2016-1904-1-BNBLK	Lab No.: M2016-1904-1
25)	Sample	✓ 8	M2016-1904-1-BN	Lab No.: M2016-1904-1
Acquisition Method: GBT092509-Delta EMV.M				
26)	Sample	✓ 8	M2016-1904-1-BNr	Lab No.: M2016-1904-1

simulate_sequence.log

Acquisition Method:	BNSB120510.M		
27) Sample	✓ 100	M2016-2037-1-BNBLK	Lab No.: M2016-2037-1
28) Sample	✓ 9	M2016-2037-1-BN	Lab No.: M2016-2037-1
Acquisition Method:	GBT092509-Delta EMV.M		
29) Sample	✓ 9	M2016-2037-1-BNr	Lab No.: M2016-2037-1
Acquisition Method:	BNSB120510.M		
30) Sample	✓ 100	M2016-2070-2-BNBLK	Lab No.: M2016-2070-2
31) Sample	✓ 10	M2016-2070-2-BN	Lab No.: M2016-2070-2
Acquisition Method:	GBT092509-Delta EMV.M		
32) Sample	✓ 10	M2016-2070-2-BNr	Lab No.: M2016-2070-2
Acquisition Method:	BNSB120510.M		
33) Sample	✓ 100	M2016-2204-2-BNBLK	Lab No.: M2016-2204-2
34) Sample	✓ 11	M2016-2204-2BN	Lab No.: M2016-2204-2
Acquisition Method:	GBT092509-Delta EMV.M		
35) Sample	✓ 11	M2016-2204-2-BNr	Lab No.: M2016-2204-2
Acquisition Method:	BNSB120510.M		
36) Sample	✓ 100	M2016-2863-2-BNBLK	Lab No.: M2016-2863-2
37) Sample	✓ 12	M2016-2863-2-BN	Lab No.: M2016-2863-2
Acquisition Method:	GBT092509-Delta EMV.M		
38) Sample	✓ 12	M2016-2863-2-BNr	Lab No.: M2016-2863-2
Acquisition Method:	BNSB120510.M		
39) Sample	✓ 100	P2016-1139-1-BNBLK	Lab No.: P2016-1139-1
40) Sample	✓ 13	P2016-1139-1-BN	Lab No.: P2016-1139-1
Acquisition Method:	GBT092509-Delta EMV.M		
41) Sample	✓ 13	P2016-1139-1-BNr	Lab No.: P2016-1139-1
Acquisition Method:	BNSB120510.M		
42) Sample	✓ 100	P2016-1174-1-BNBLK	Lab No.: P2016-1174-1
43) Sample	✓ 14	P2016-1174-1-BN	Lab No.: P2016-1174-1
Acquisition Method:	GBT092509-Delta EMV.M		
44) Sample	✓ 14	P2016-1174-1-BNr	Lab No.: P2016-1174-1
Acquisition Method:	BNSB120510.M		
45) Sample	✓ 100	P2016-1184-1-BNBLK	Lab No.: P2016-1184-1
46) Sample	✓ 15	P2016-1184-1-BN	Lab No.: P2016-1184-1
Acquisition Method:	GBT092509-Delta EMV.M		
47) Sample	✓ 15	P2016-1184-1-BNr	Lab No.: P2016-1184-1
Acquisition Method:	BNSB120510.M		
48) Sample	✓ 99	P2016-1191-1-BNBLK	Lab No.: P2016-1191-1
49) Sample	✓ 16	P2016-1191-1-BN	Lab No.: P2016-1191-1
Acquisition Method:	GBT092509-Delta EMV.M		
50) Sample	✓ 16	P2016-1191-1-BNr	Lab No.: P2016-1191-1
Acquisition Method:	BNSB120510.M		
51) Sample	✓ 99	P2016-1205-2-BNBLK	Lab No.: P2016-1205-2
52) Sample	✓ 17	P2016-1205-2-BN	Lab No.: P2016-1205-2
Acquisition Method:	GBT092509-Delta EMV.M		
53) Sample	✓ 17	P2016-1205-2-BNr	Lab No.: P2016-1205-2
Acquisition Method:	BNSB120510.M		
54) Sample	✓ 99	P2016-1206-1-BNBLK	Lab No.: P2016-1206-1
55) Sample	✓ 18	P2016-1206-1-BN	Lab No.: P2016-1206-1

simulate_sequence.log


Acquisition Method: GBT092509-Delta EMV.M			
56) Sample ✓ 18	P2016-1206-1-BNr	Lab No.:	P2016-1206-1
Acquisition Method: BNSB120510.M			
57) Sample ✓ 99	P2016-1209-1-BNBLK	Lab No.:	P2016-1209-1
58) Sample ✓ 19	P2016-1209-1-BN	Lab No.:	P2016-1209-1
Acquisition Method: GBT092509-Delta EMV.M			
59) Sample ✓ 19	P2016-1209-1-BNr	Lab No.:	P2016-1209-1
Acquisition Method: BNSB120510.M			
60) Sample ✓ 99	P2016-1210-1-BNBLK	Lab No.:	P2016-1210-1
61) Sample ✓ 20	P2016-1210-1-BN	Lab No.:	P2016-1210-1
Acquisition Method: GBT092509-Delta EMV.M			
62) Sample ✓ 20	P2016-1210-1-BNr	Lab No.:	P2016-1210-1
Acquisition Method: BNSB120510.M			
63) Sample ✓ 99	P2016-1211-1-BNBLK	Lab No.:	P2016-1211-1
64) Sample ✓ 21	P2016-1211-1-BN	Lab No.:	P2016-1211-1
Acquisition Method: GBT092509-Delta EMV.M			
65) Sample ✓ 21	P2016-1211-1-BNr	Lab No.:	P2016-1211-1
Acquisition Method: BNSB120510.M			
66) Sample ✓ 99	P2016-1212-1-BNBLK	Lab No.:	P2016-1212-1
67) Sample ✓ 22	P2016-1212-1-BN	Lab No.:	P2016-1212-1
Acquisition Method: GBT092509-Delta EMV.M			
68) Sample ✓ 22	P2016-1212-1-BNr	Lab No.:	P2016-1212-1
Acquisition Method: BNSB120510.M			
69) Sample ✓ 99	P2016-1214-1-BNBLK	Lab No.:	P2016-1214-1
70) Sample ✓ 23	P2016-1214-1-BN	Lab No.:	P2016-1214-1
Acquisition Method: GBT092509-Delta EMV.M			
71) Sample ✓ 23	P2016-1214-1-BNr	Lab No.:	P2016-1214-1
Acquisition Method: BNSB120510.M			
72) Sample ✓ 99	P2016-1301-1-BNBLK	Lab No.:	P2016-1301-1
73) Sample ✓ 24	P2016-1301-1-BN	Lab No.:	P2016-1301-1
Acquisition Method: GBT092509-Delta EMV.M			
74) Sample ✓ 24	P2016-1301-1-BNr	Lab No.:	P2016-1301-1
Acquisition Method: BNSB120510.M			
75) Sample ✓ 99	P2016-1327-1-BNBLK	Lab No.:	P2016-1327-1
76) Sample ✓ 25	P2016-1327-1-BN	Lab No.:	P2016-1327-1
Acquisition Method: GBT092509-Delta EMV.M			
77) Sample ✓ 25	P2016-1327-1-BNr	Lab No.:	P2016-1327-1
Acquisition Method: BNSB120510.M			
78) Sample ✓ 99	P2016-1359-1-BNBLK	Lab No.:	P2016-1359-1
79) Sample ✓ 26	P2016-1359-1-BN	Lab No.:	P2016-1359-1
Acquisition Method: GBT092509-Delta EMV.M			
80) Sample ✓ 26	P2016-1359-1-BNr	Lab No.:	P2016-1359-1
Acquisition Method: BNSB120510.M			
81) Sample ✓ 99	P2016-1582-1-BNBLK	Lab No.:	P2016-1582-1
82) Sample ✓ 27	P2016-1582-1-BN	Lab No.:	P2016-1582-1
Acquisition Method: GBT092509-Delta EMV.M			
83) Sample ✓ 27	P2016-1582-1-BNr	Lab No.:	P2016-1582-1
Acquisition Method: BNSB120510.M			
84) Sample ✓ 99	POSTBLK	BLK	

simulate_sequence.log


Acquisition Method: GBT092509-Delta EMV.M
85) Sample 99 AFTER
megabytes Needed: 870 Space on drive D: 218628
Sequence Verification Done!

BLK


File : F:\10052016\10052016\Prerun Solvent Blank.D
Operator : ISP\datastor
Acquired : 05 Oct 2016 11:27 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Pre-run Solvent Blank
Misc Info : Chloroform
Vial Number: 100

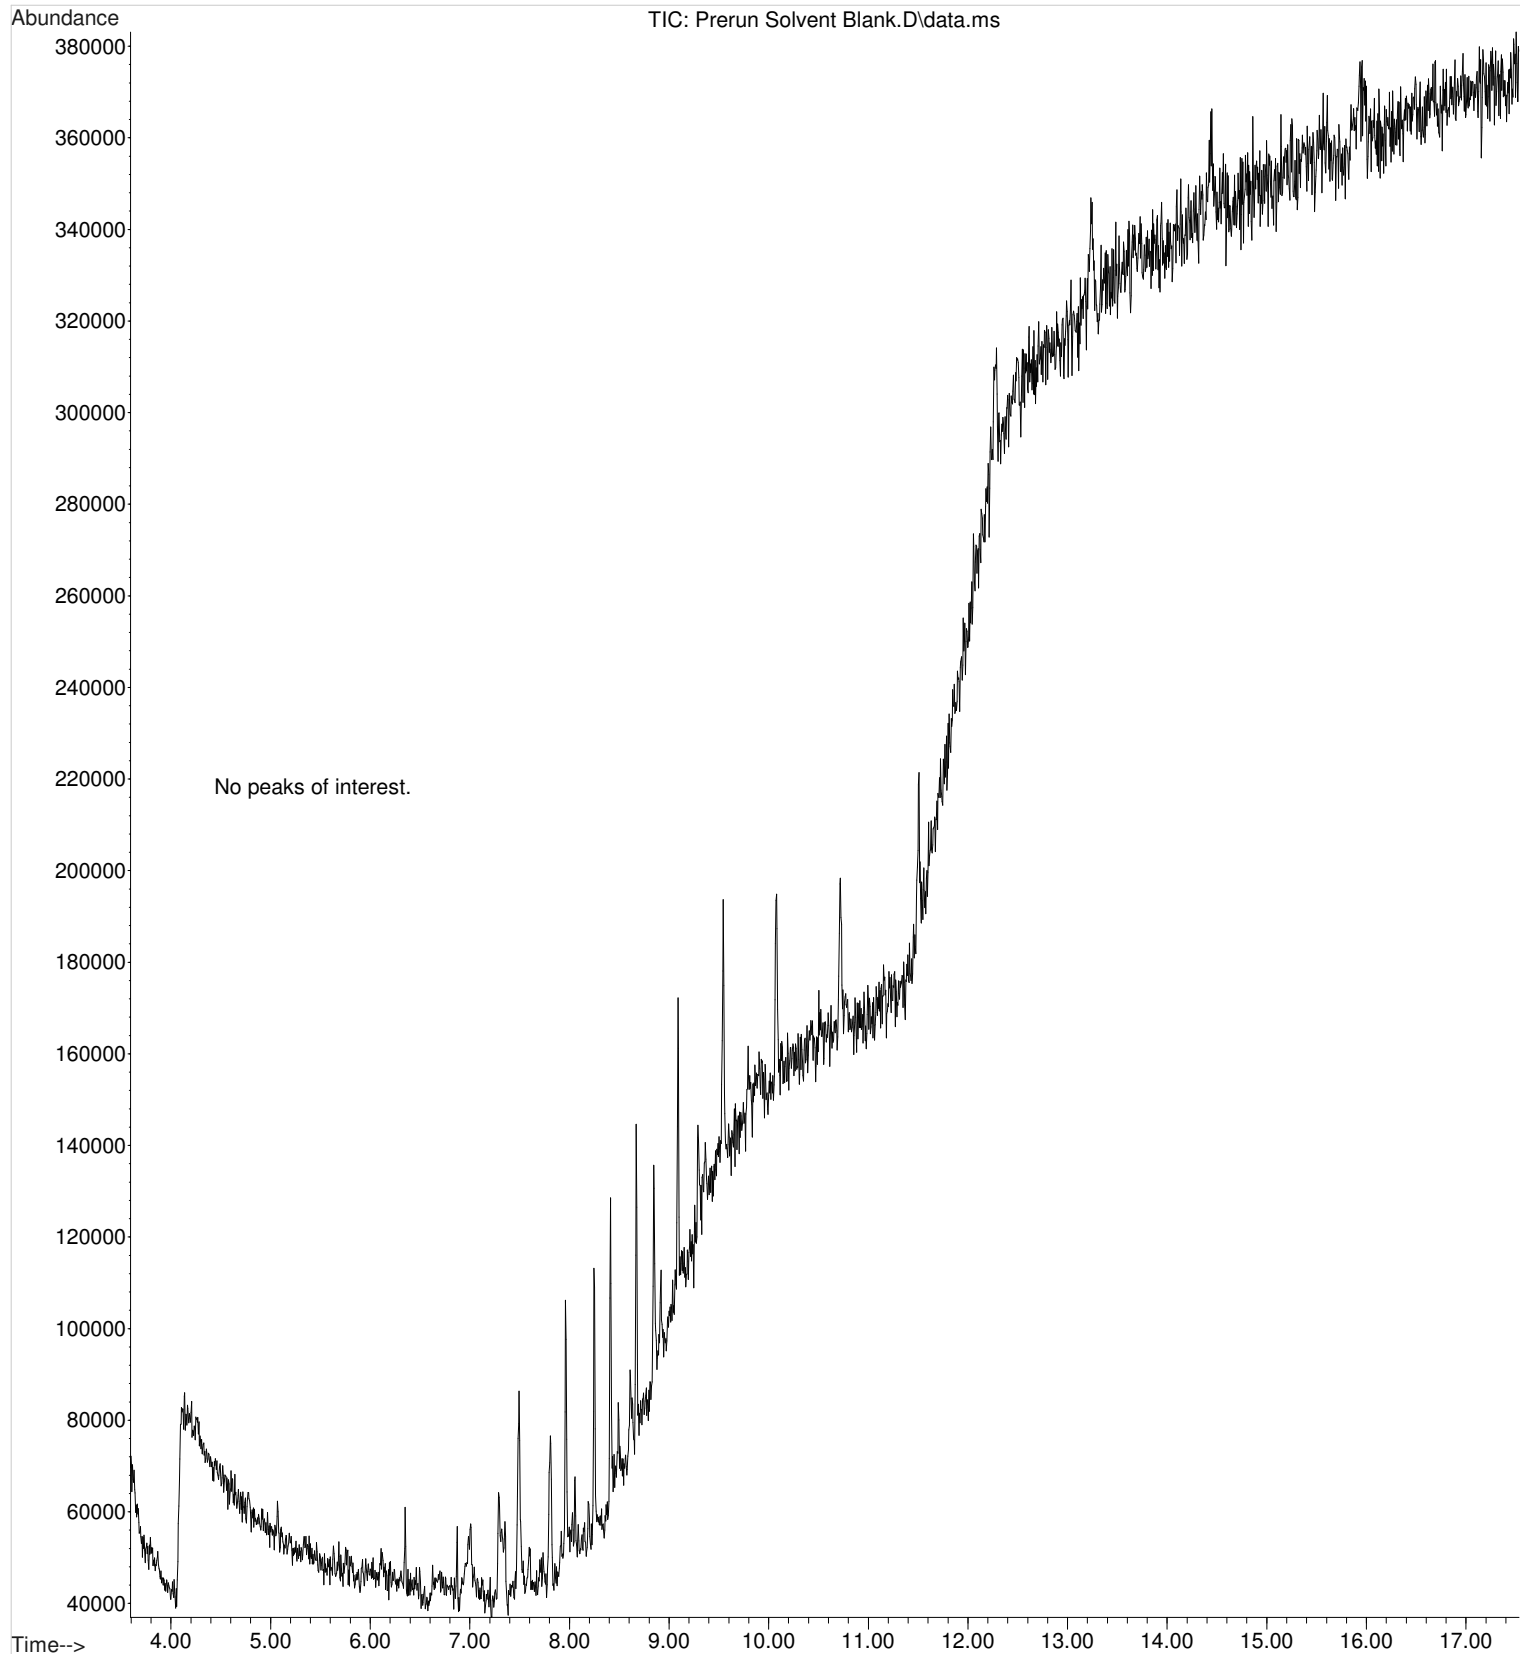



File : F:\10052016\10052016\10052016\prbLK2.D
Operator : ISP\datastor
Acquired : 05 Oct 2016 12:36 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Solvent Blank
Misc Info : Chloroform
Vial Number: 99

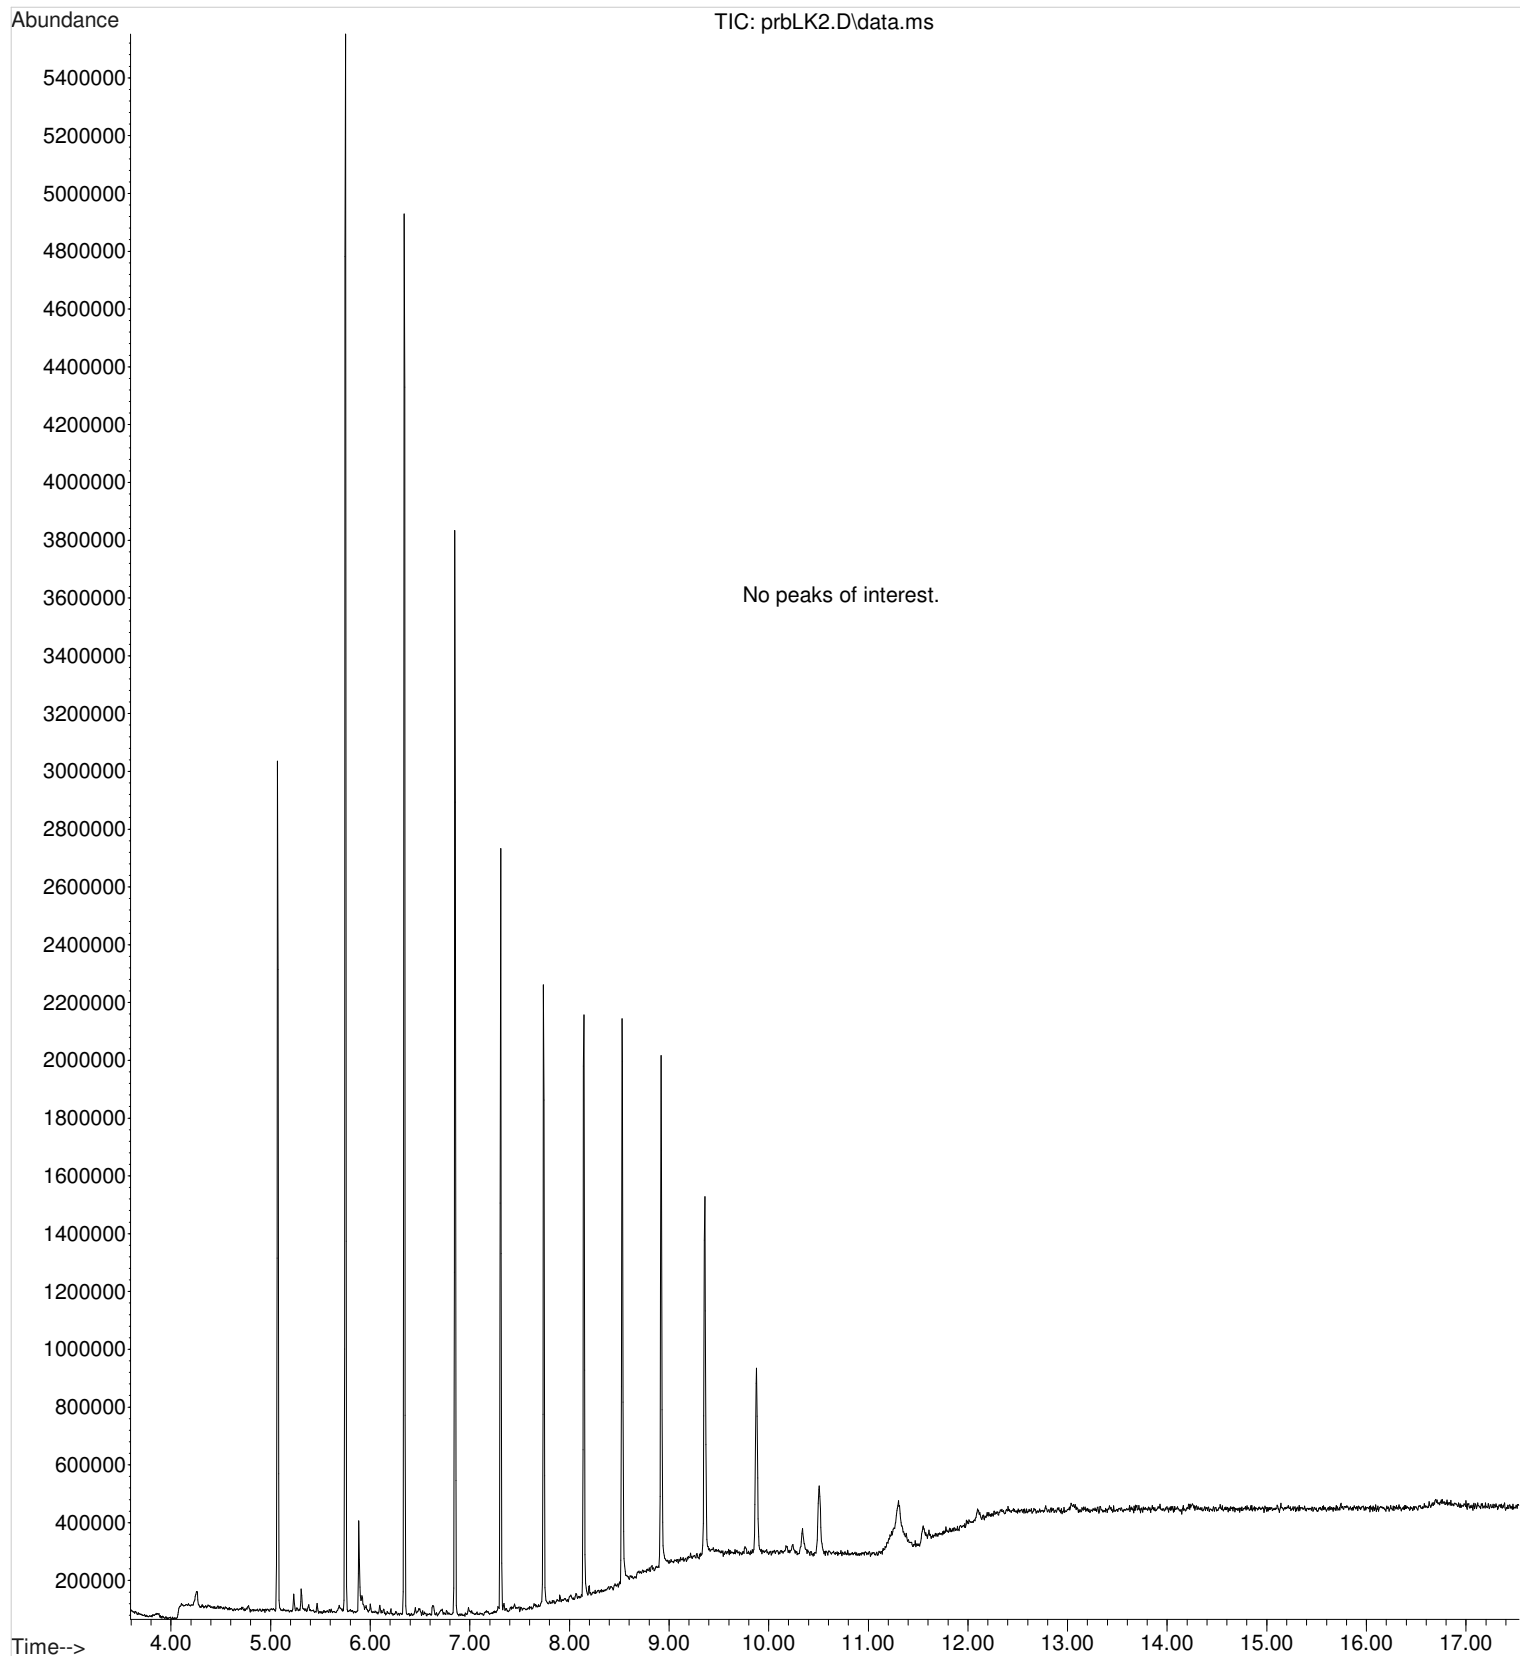



File :F:\10052016\10052016\Negative Control-BN.D
Operator : ISP\datastor
Acquired : 05 Oct 2016 11:50 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B1013
Misc Info : Analytical Method 3.6.1
Vial Number: 1

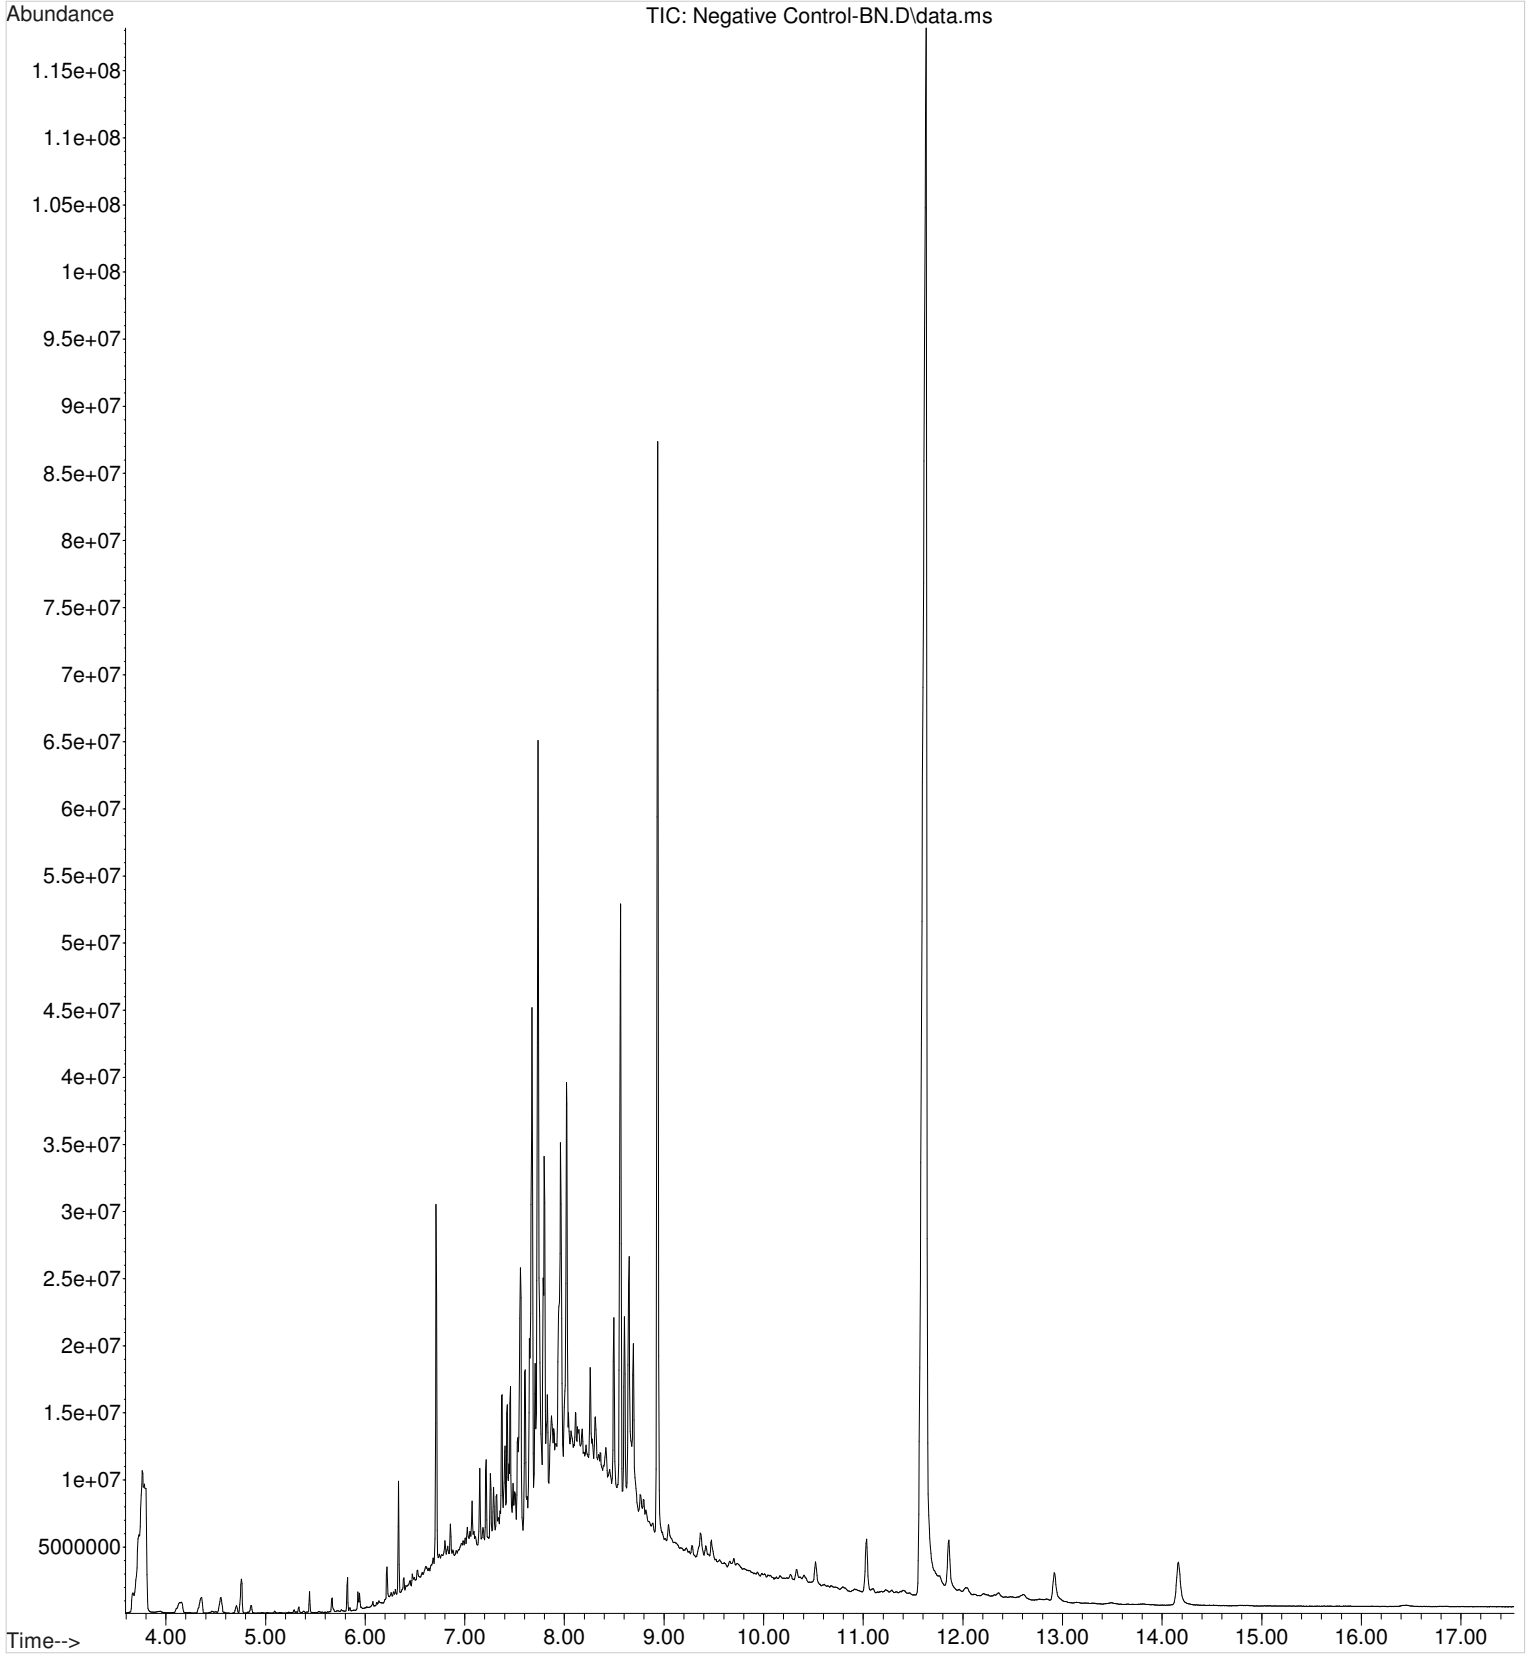

File : F:\10052016\10052016\Negative Control-BN.D
Operator : ISP\datastor
Acquired : 05 Oct 2016 11:50 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name : Negative Control - Utak Lot B1013
Misc Info : Analytical Method 3.6.1
Vial Number: 1

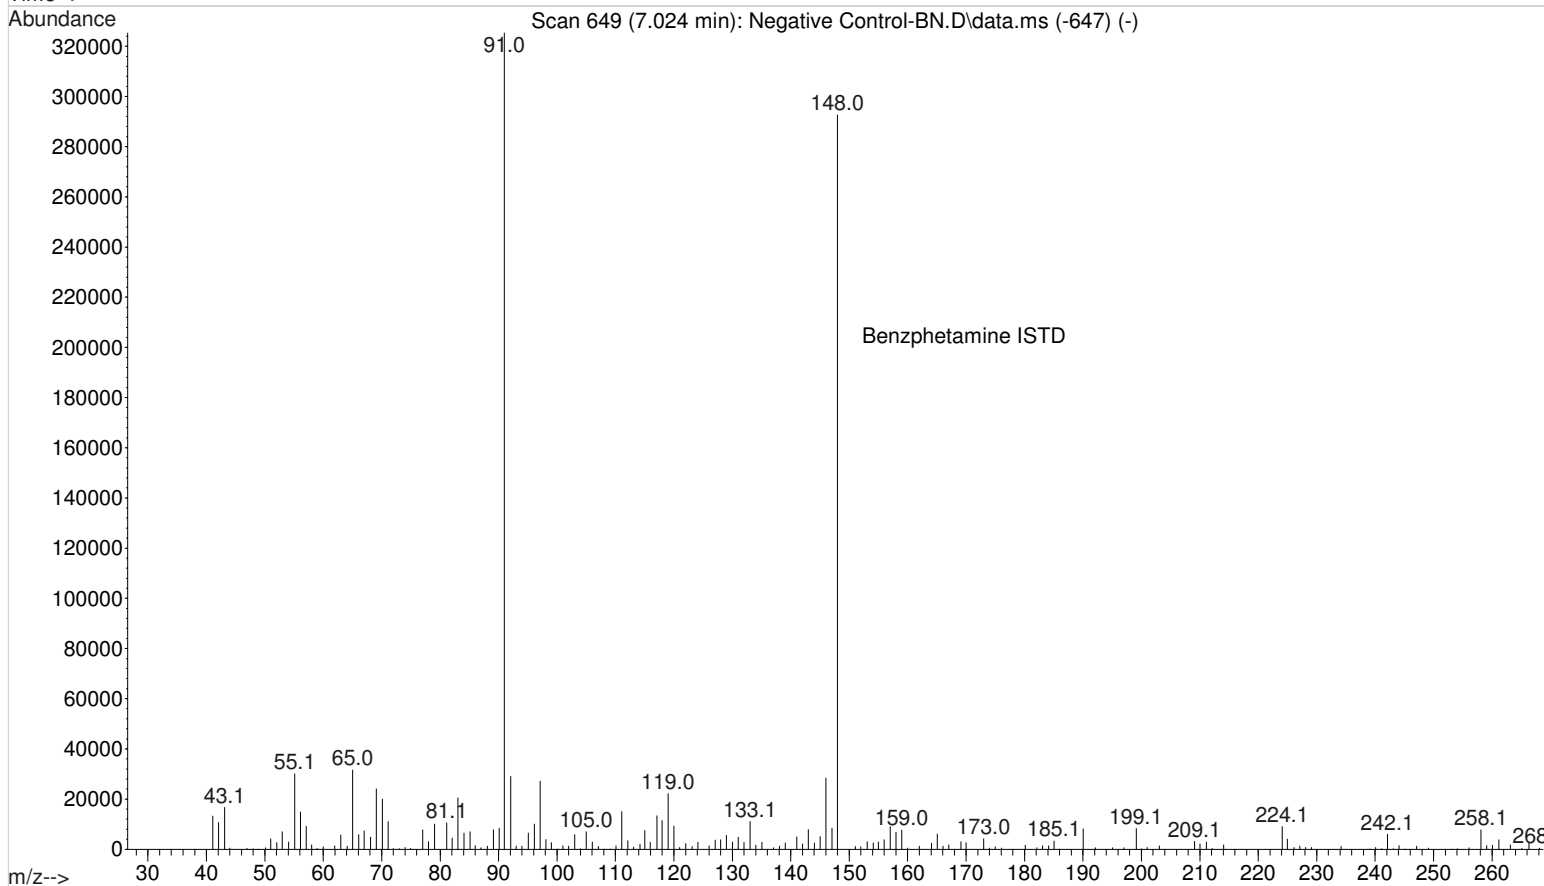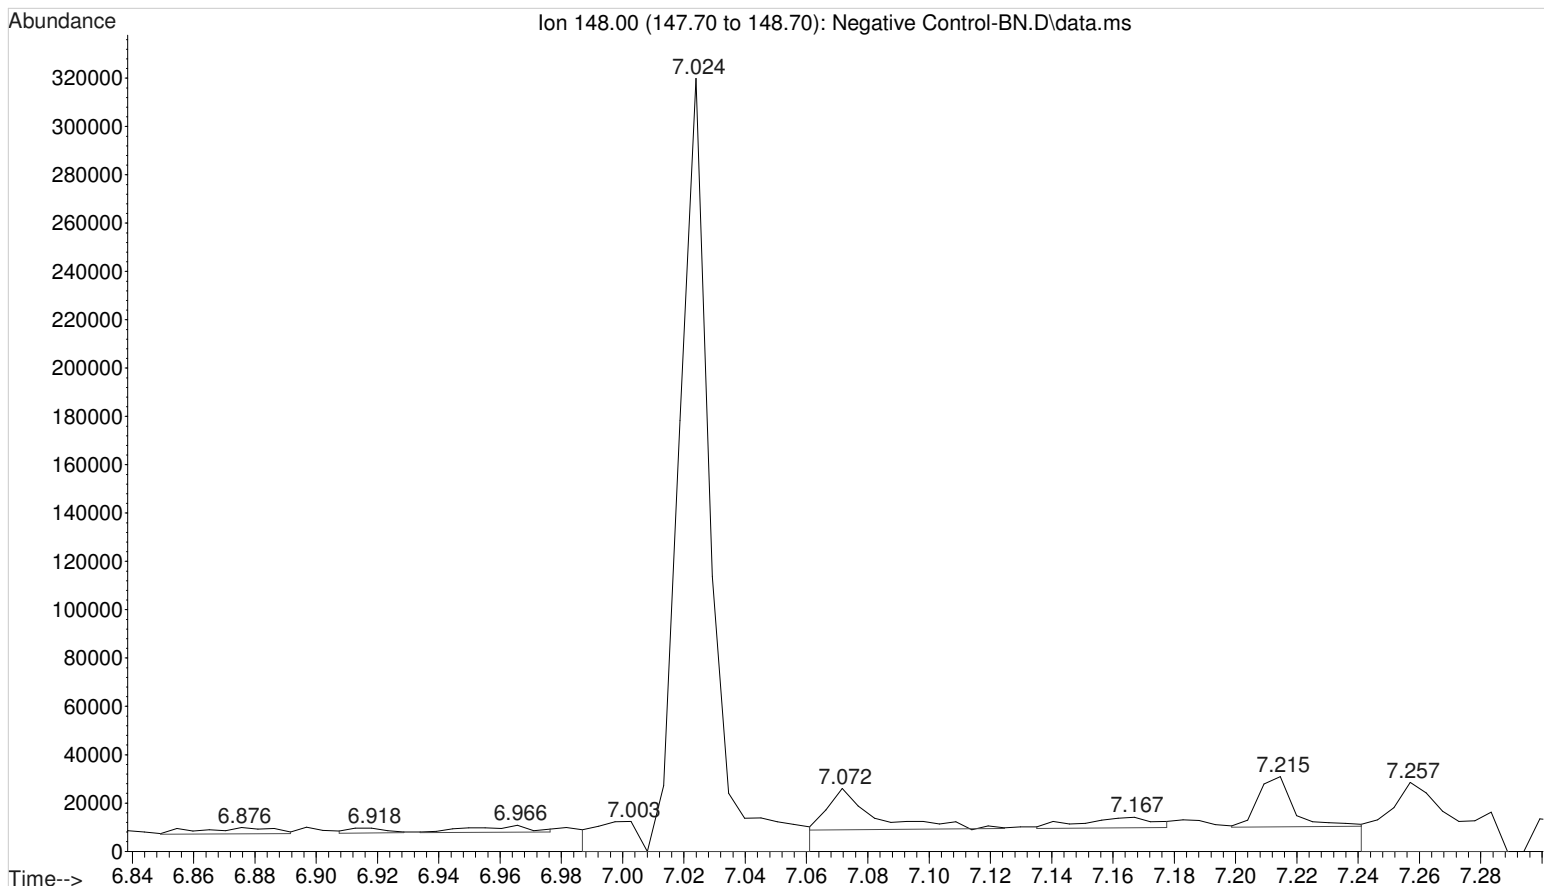


File : F:\10052016\10052016\Negative Control-BN.D
Operator : ISP\datastor
Acquired : 05 Oct 2016 11:50 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name : Negative Control - Utak Lot B1013
Misc Info : Analytical Method 3.6.1
Vial Number: 1

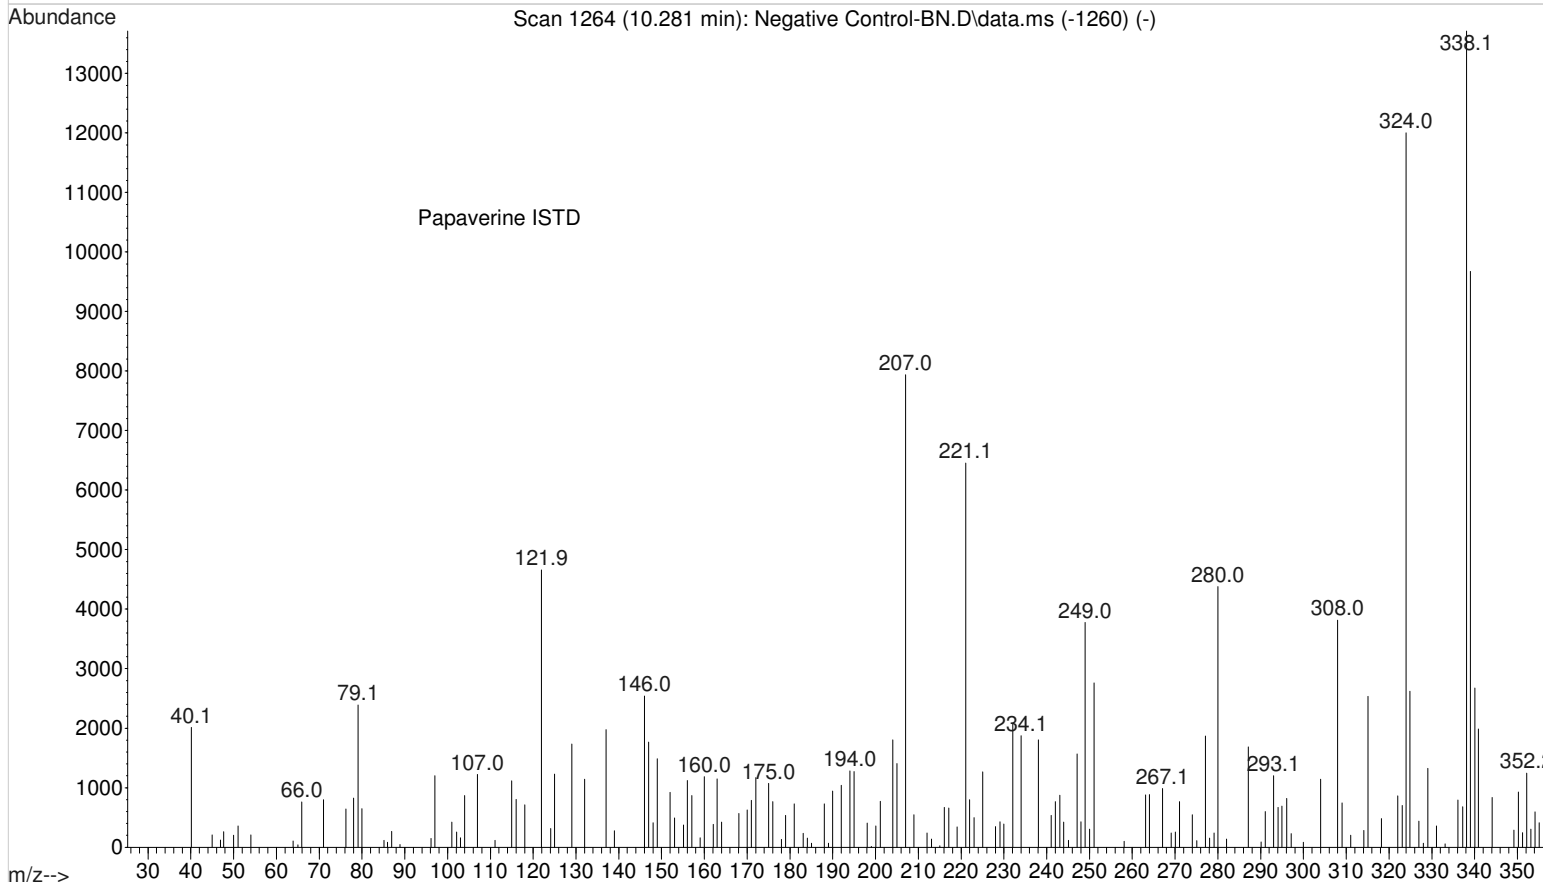
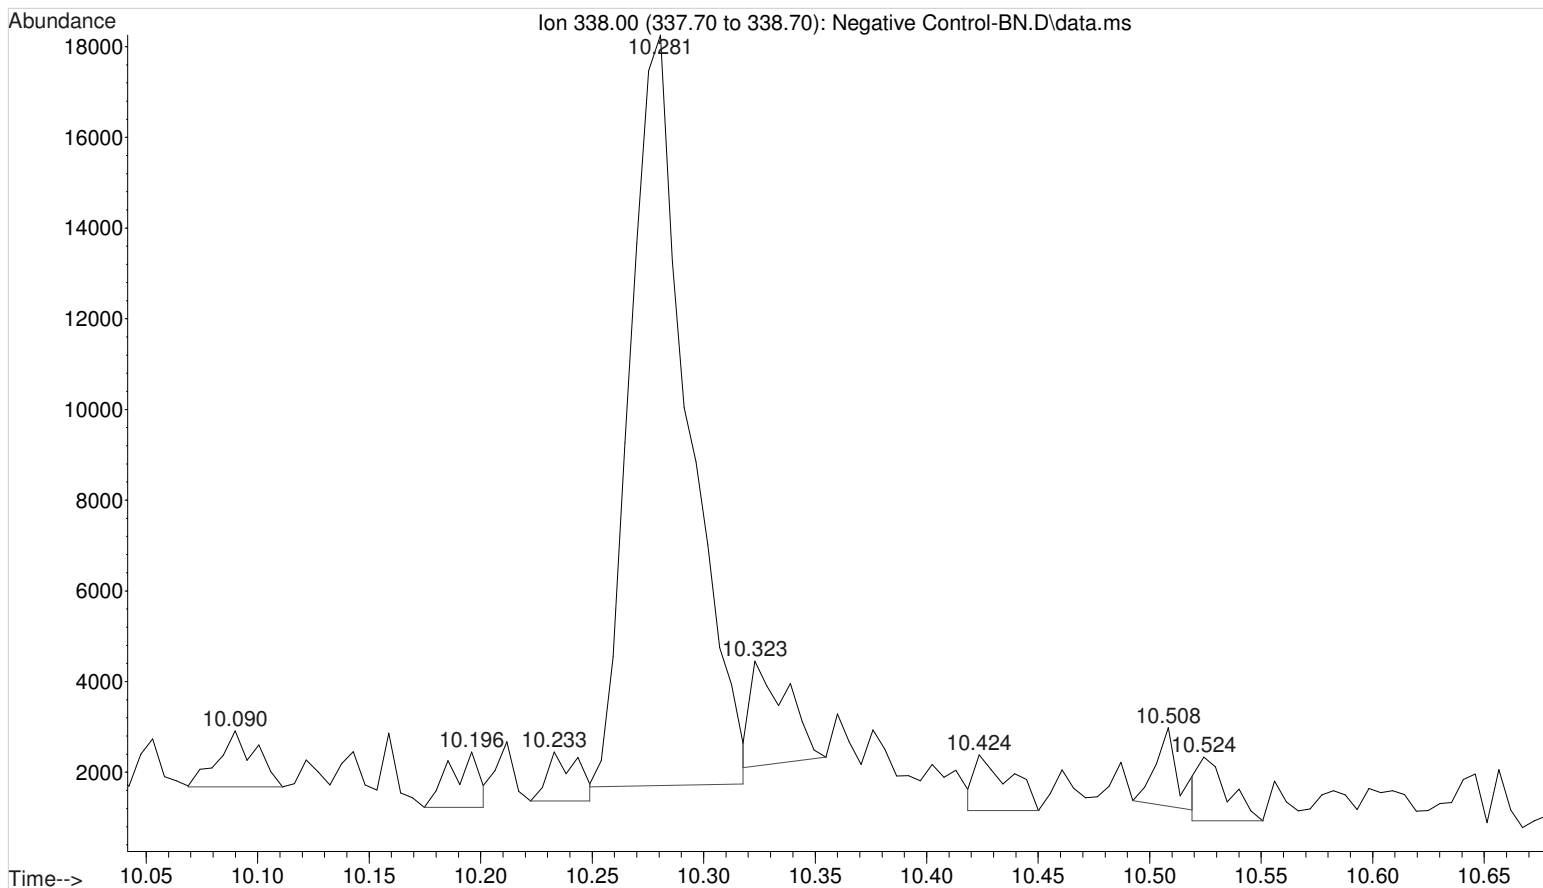


Handwritten signature



File :F:\10052016\10052016\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 05 Oct 2016 12:13 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

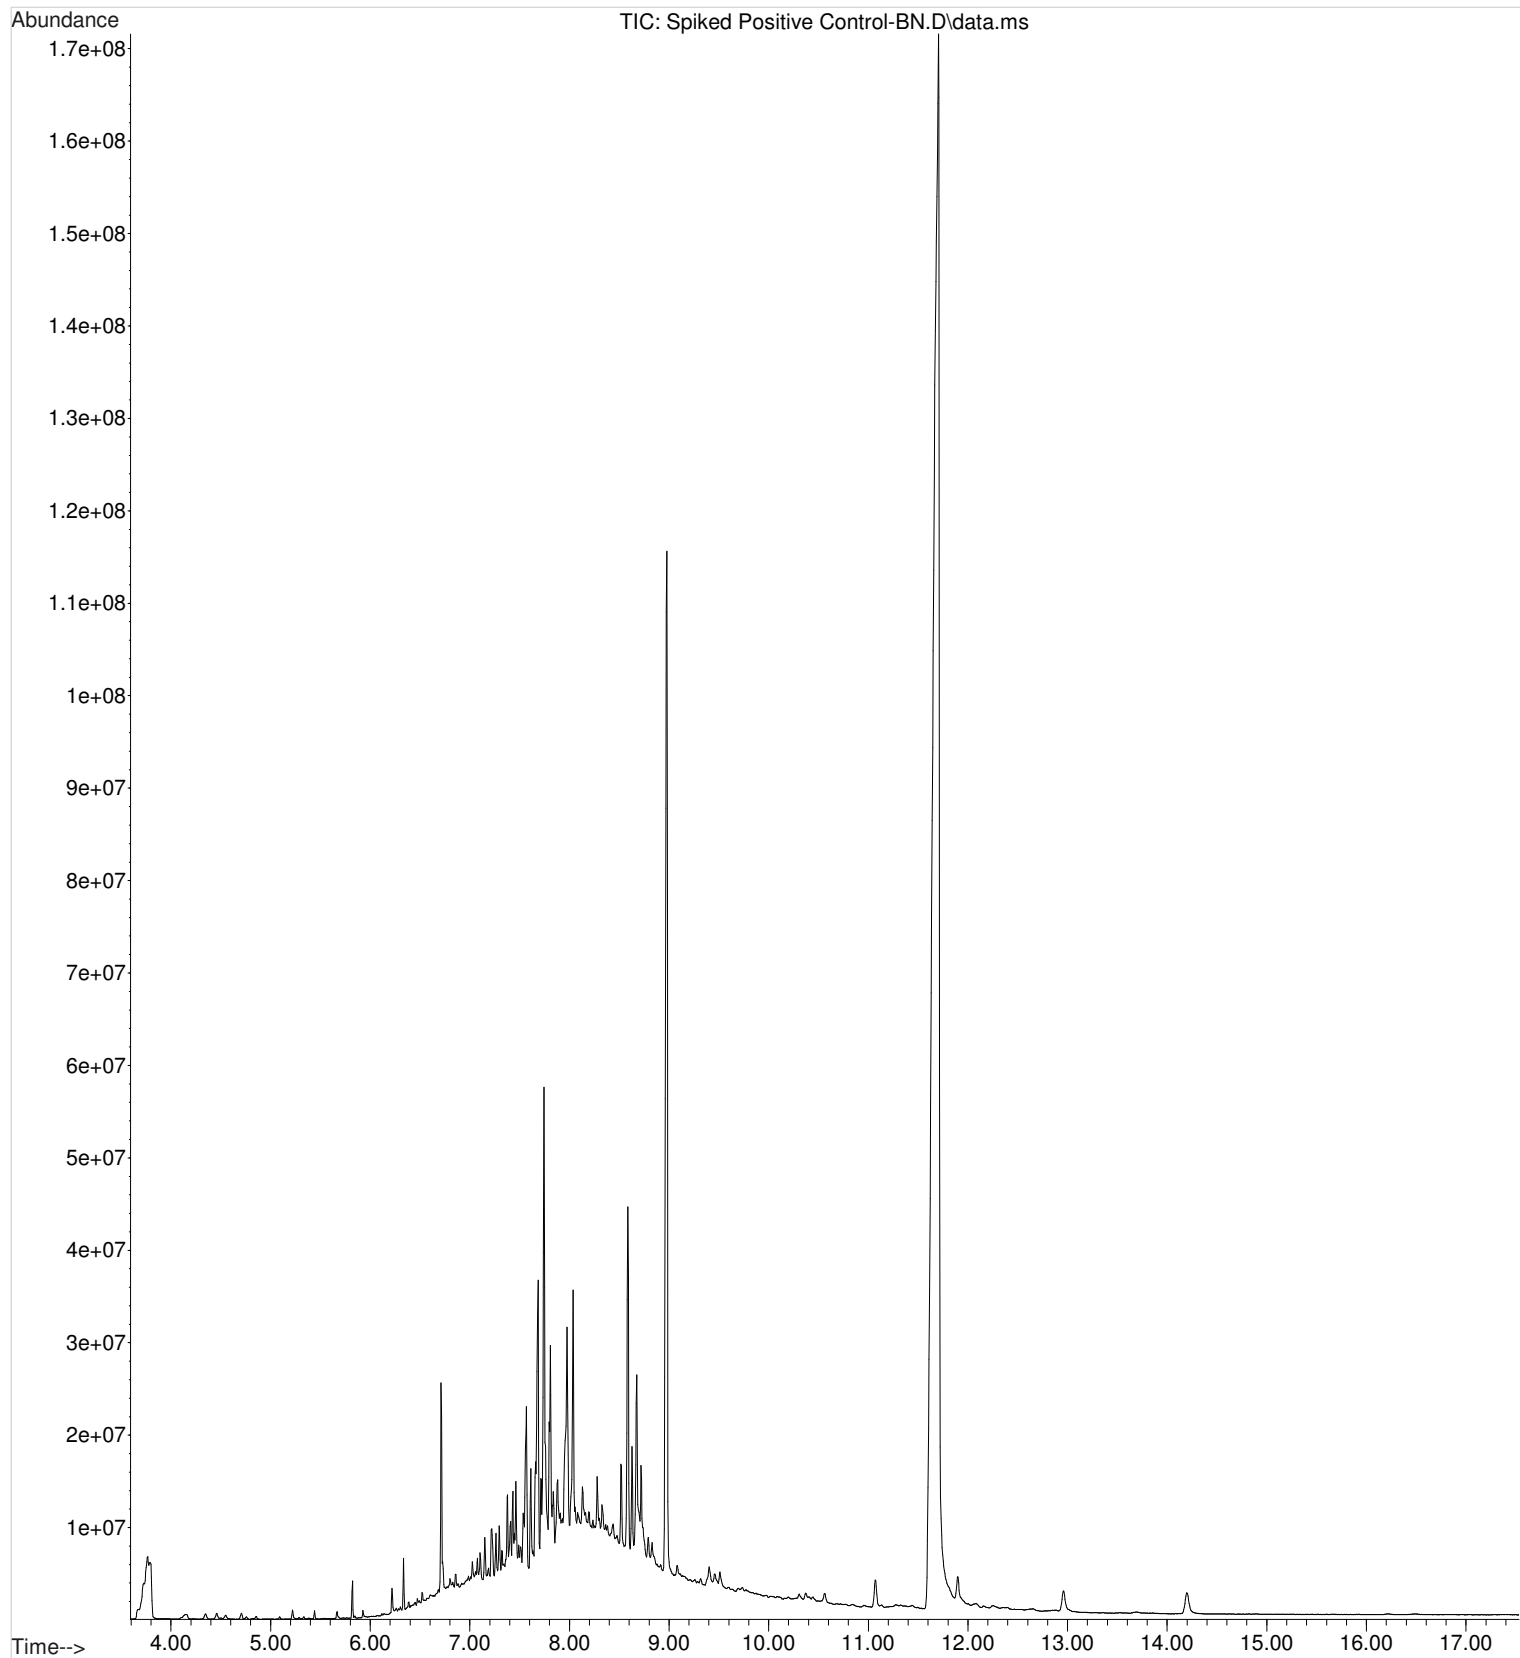



File : F:\10052016\10052016\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 05 Oct 2016 12:13 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name : Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

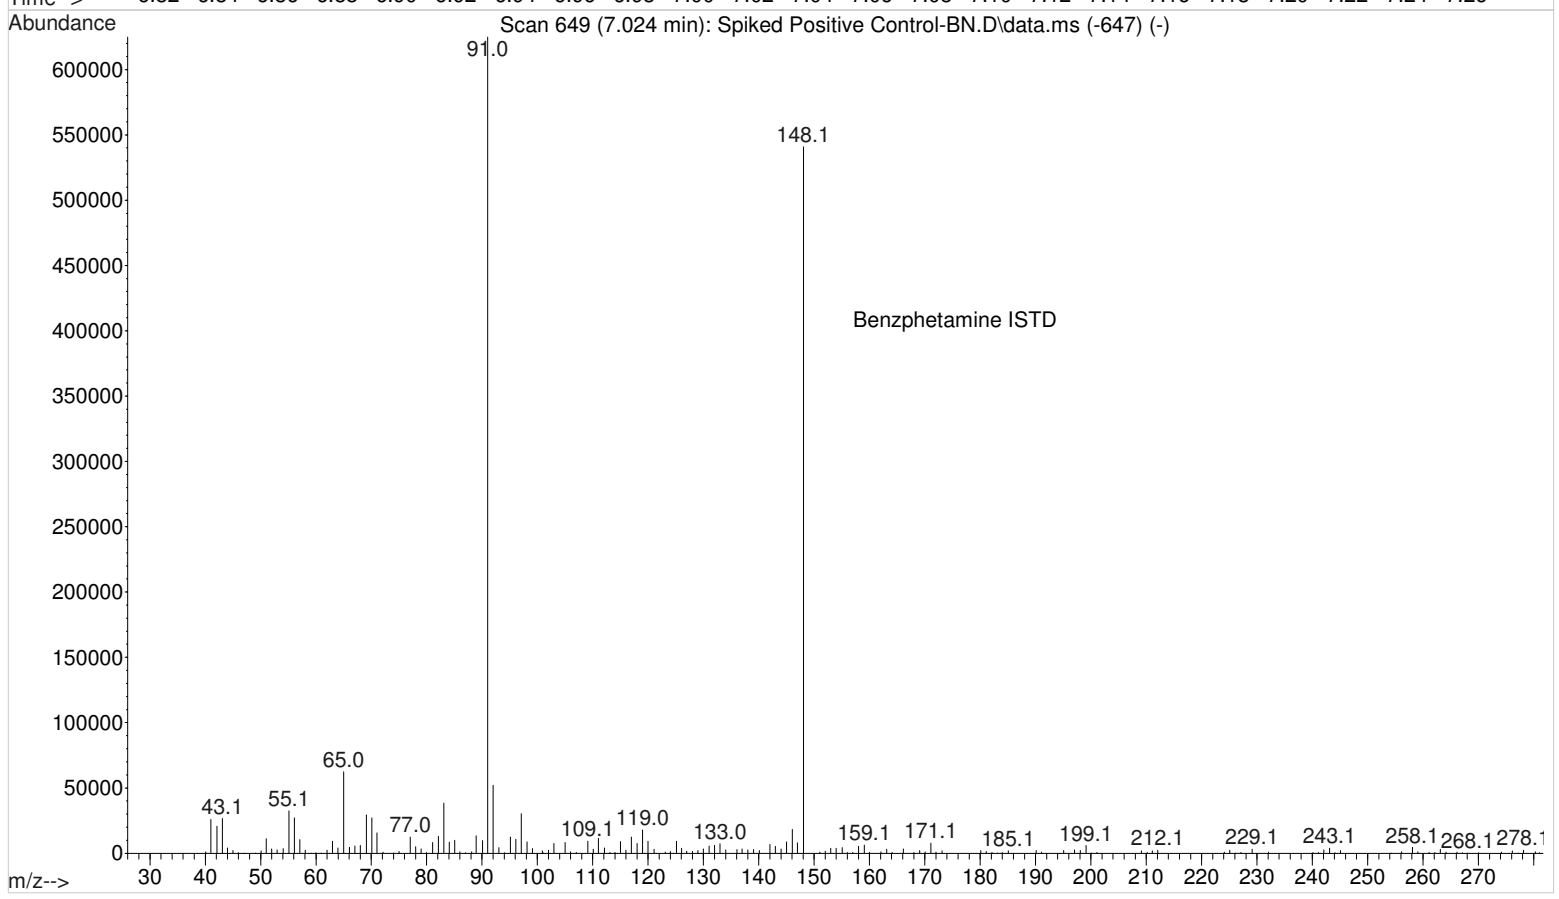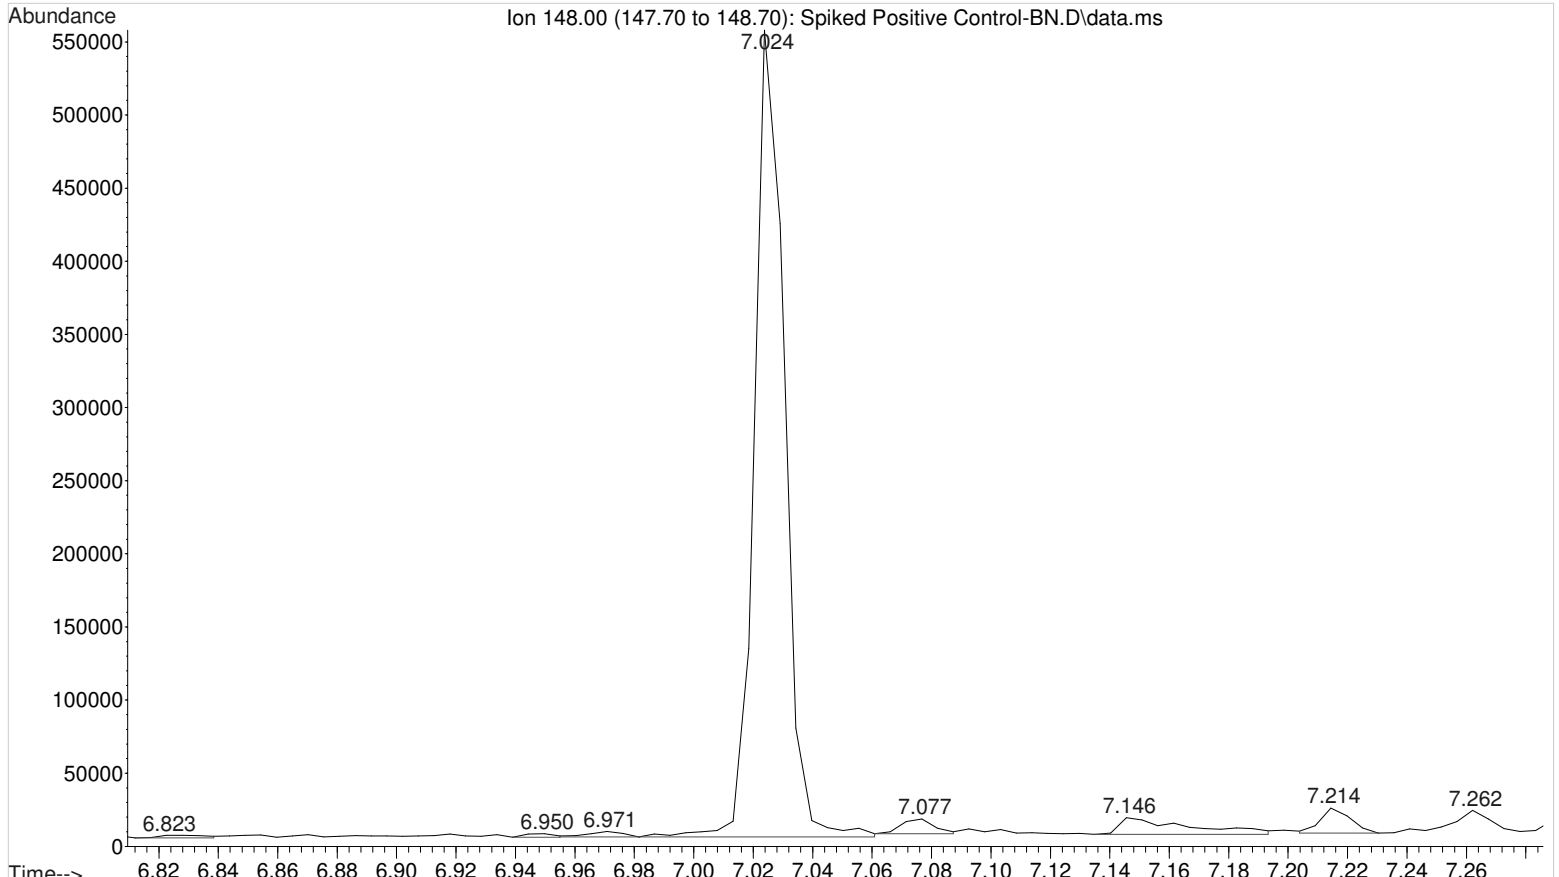



File : F:\10052016\10052016\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 05 Oct 2016 12:13 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name : Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

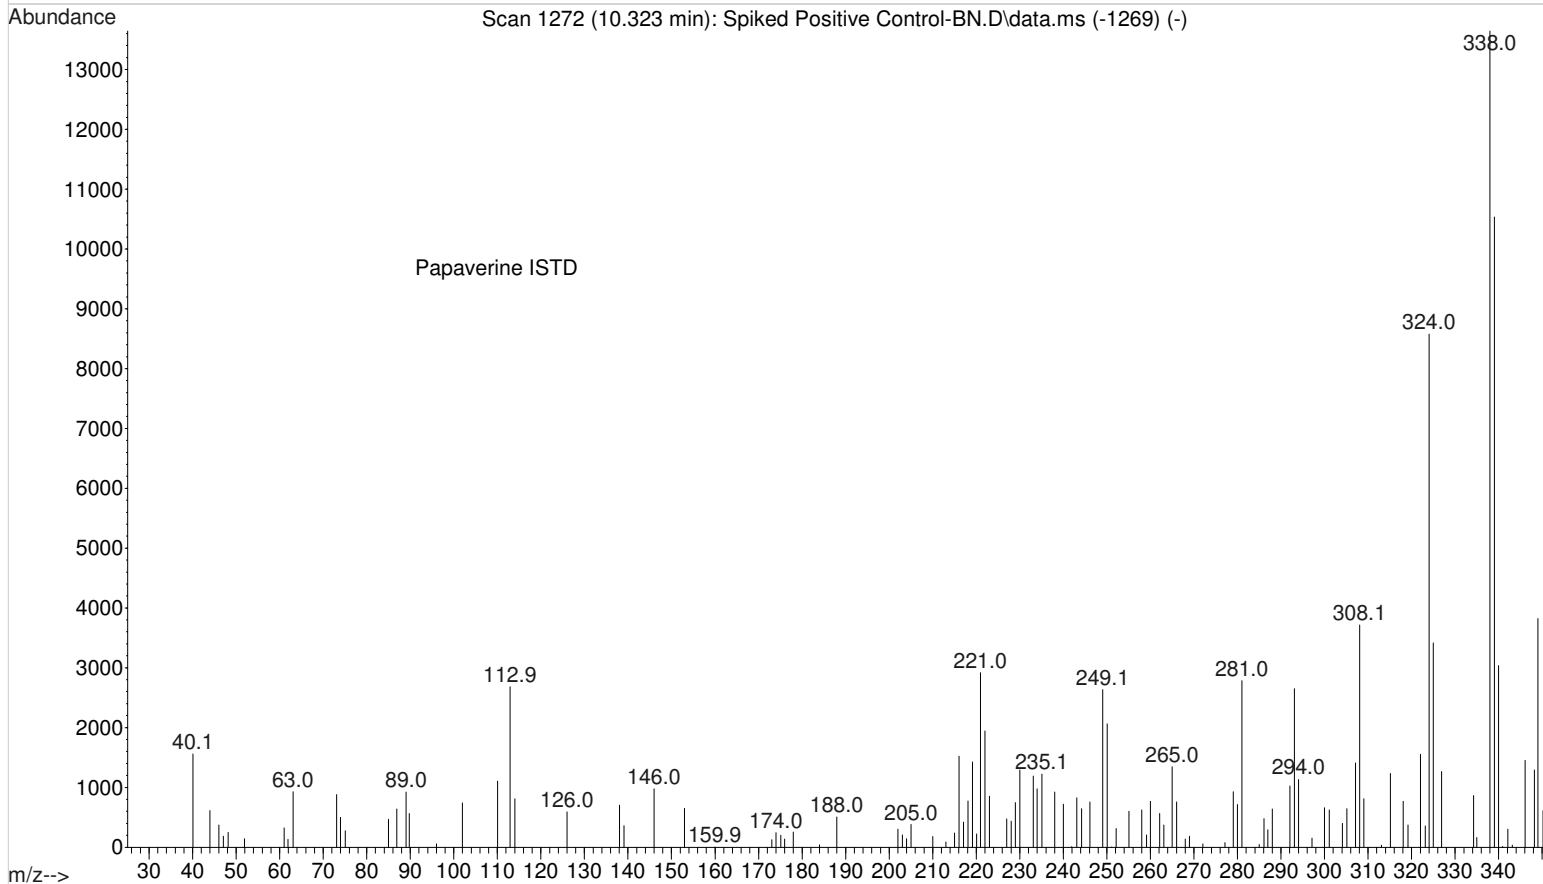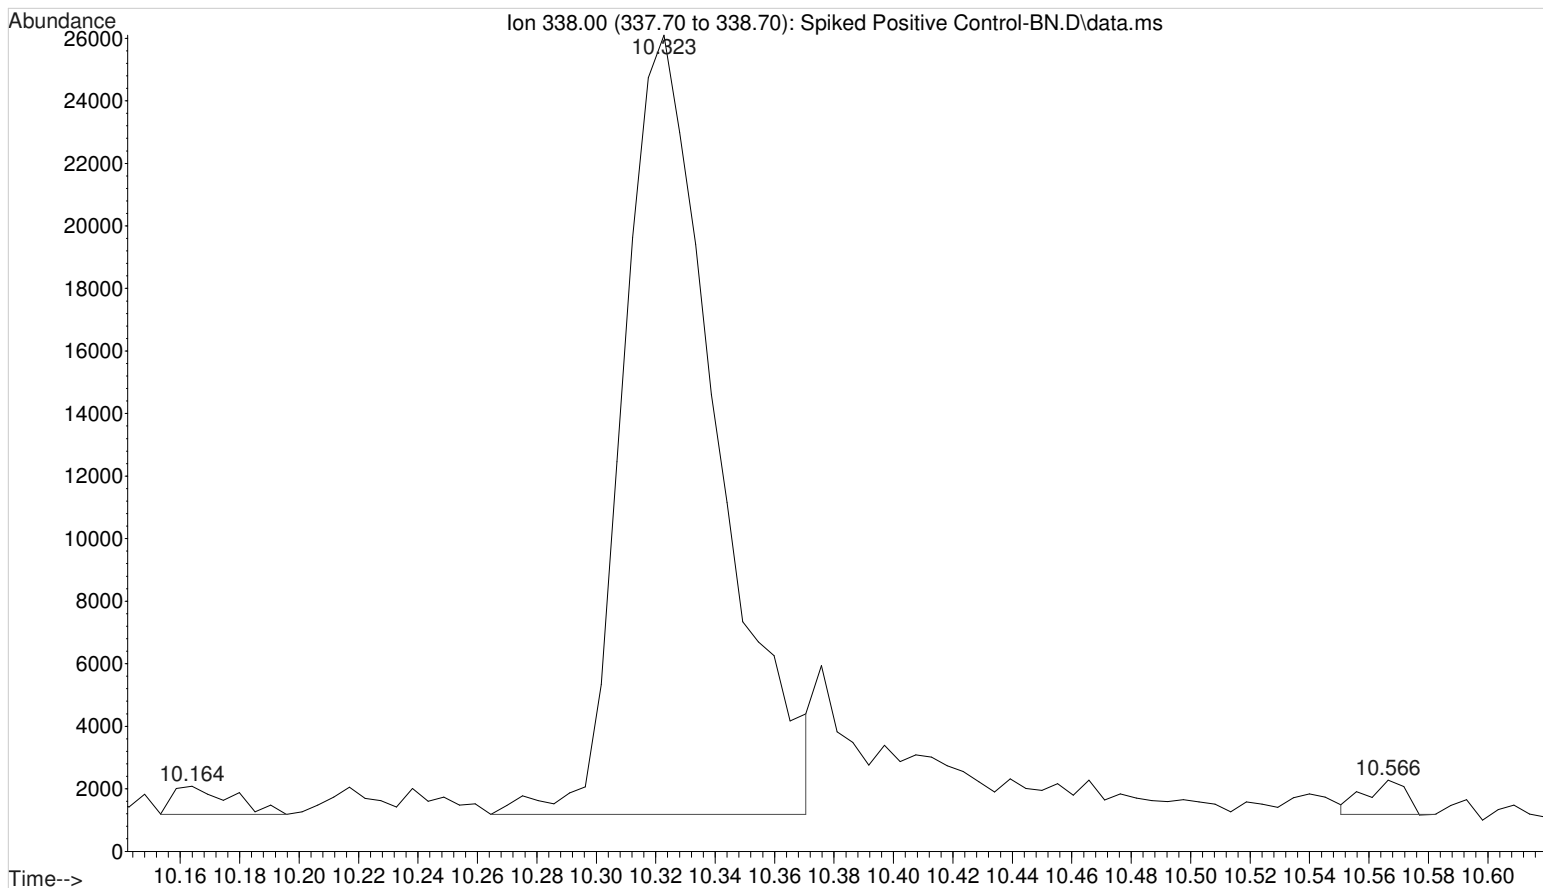



File :F:\10052016\10052016\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 05 Oct 2016 12:13 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

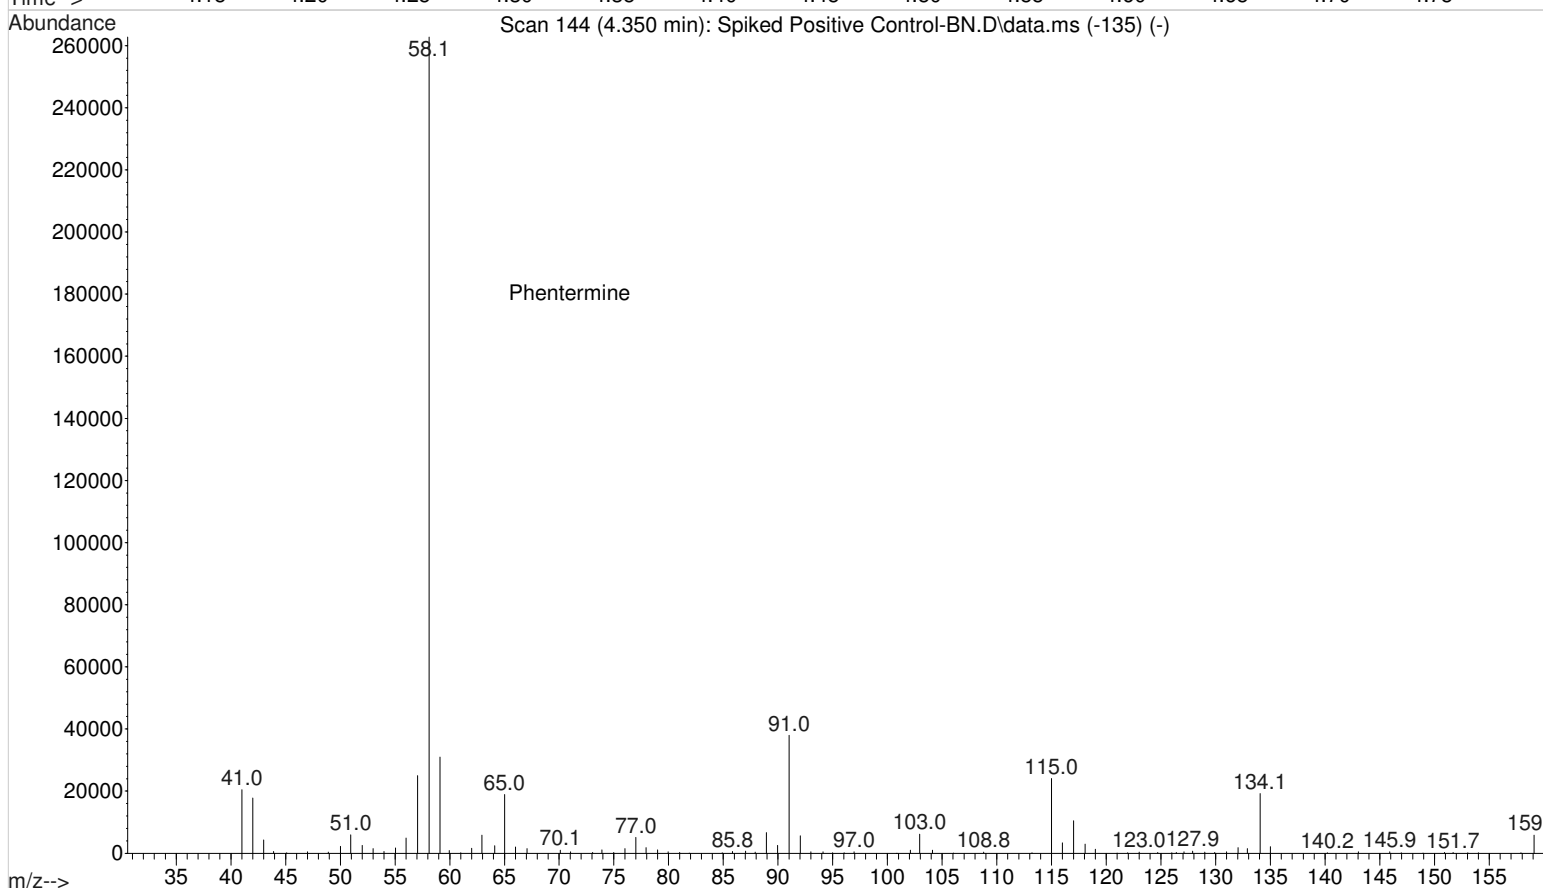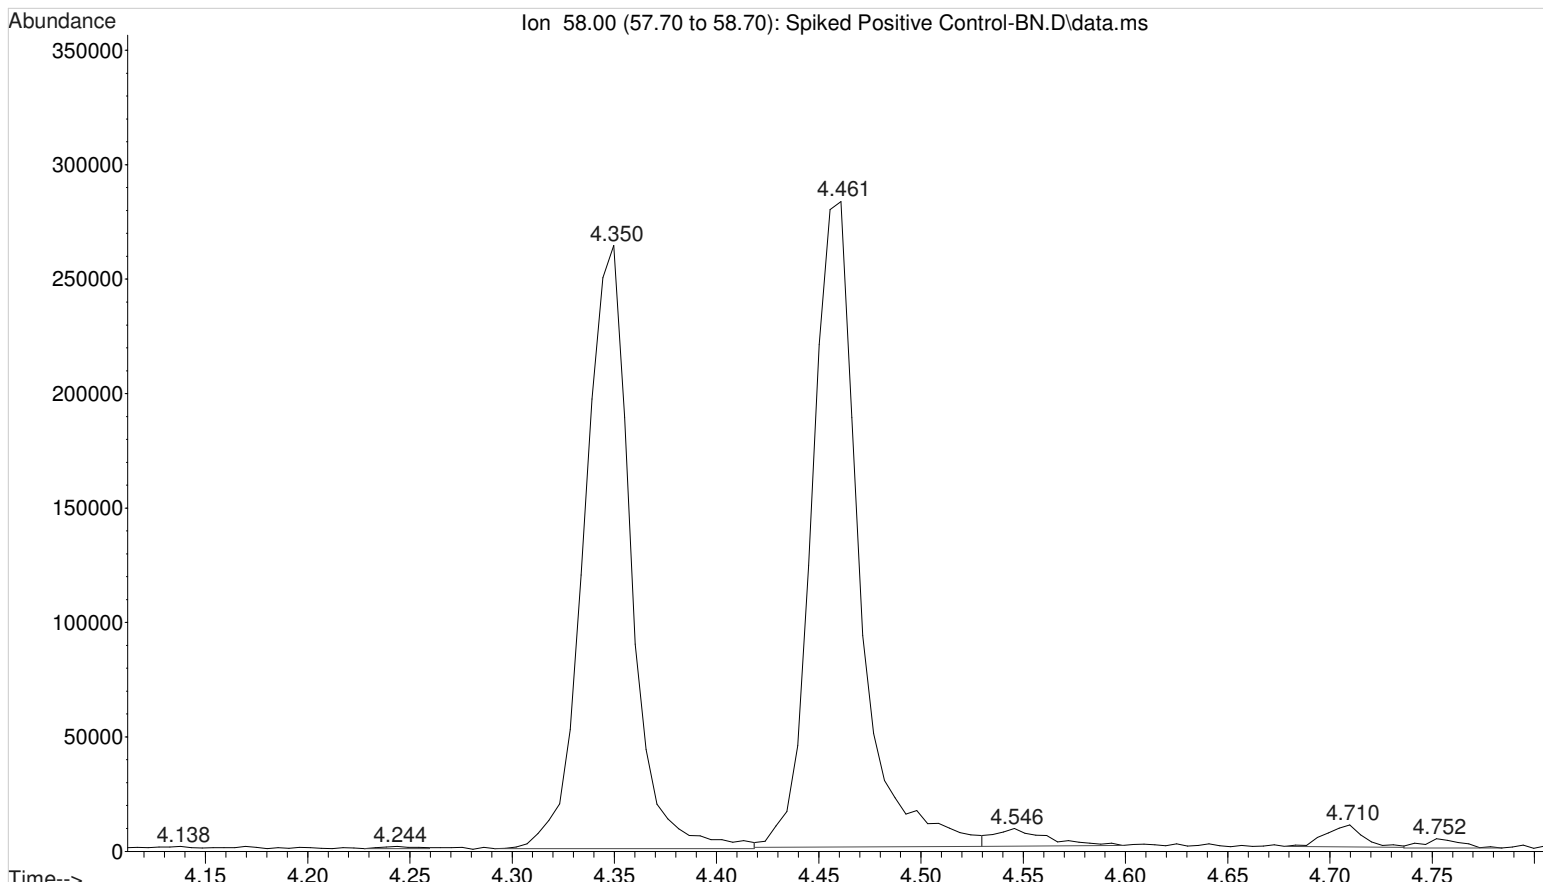



File : F:\10052016\10052016\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 05 Oct 2016 12:13 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

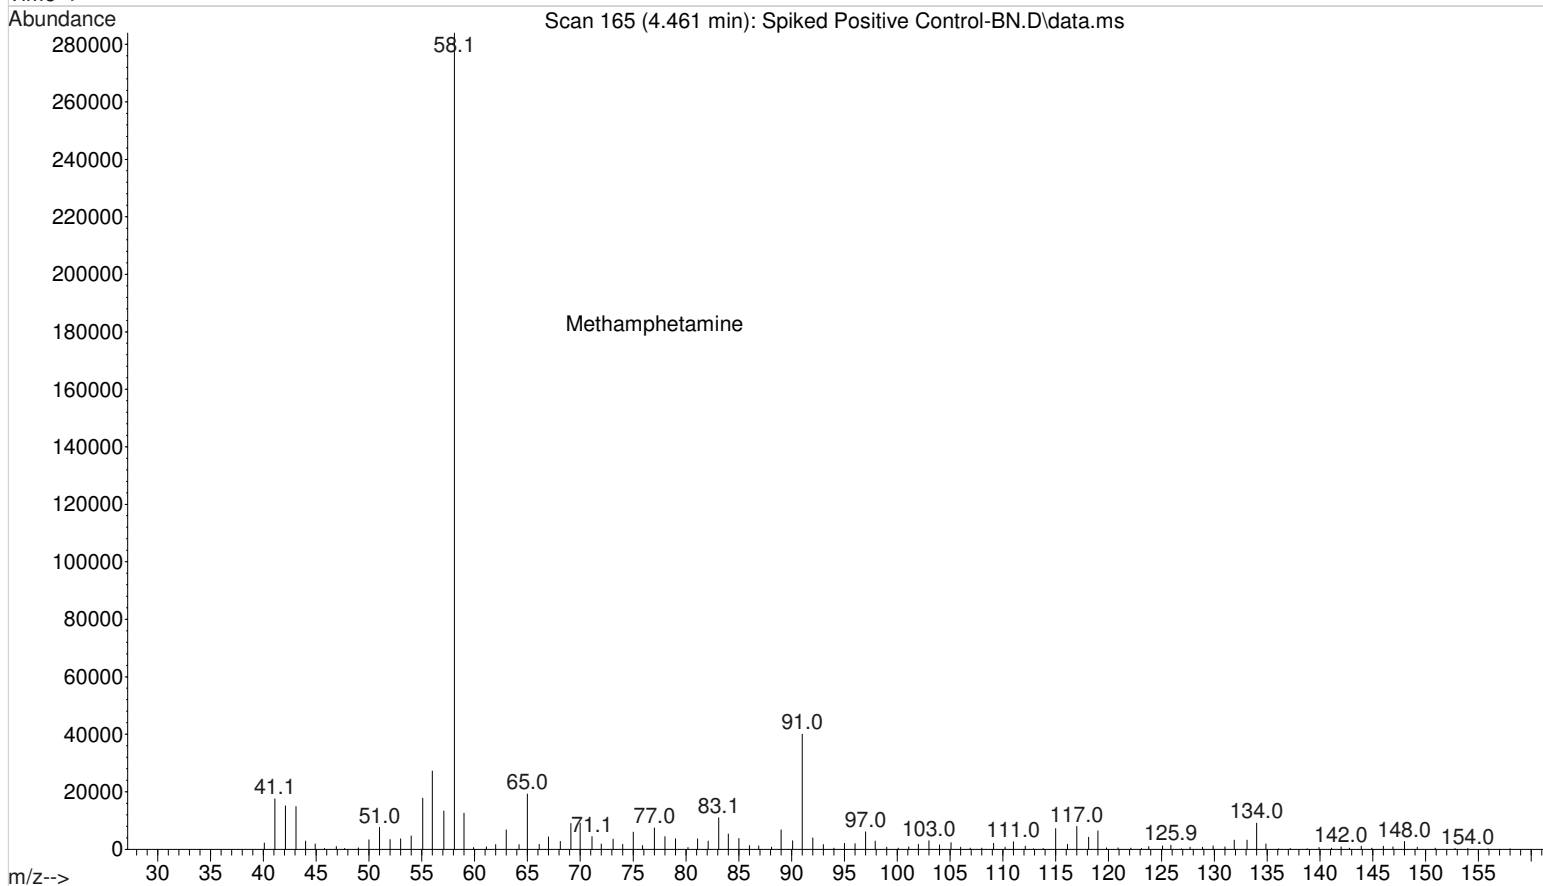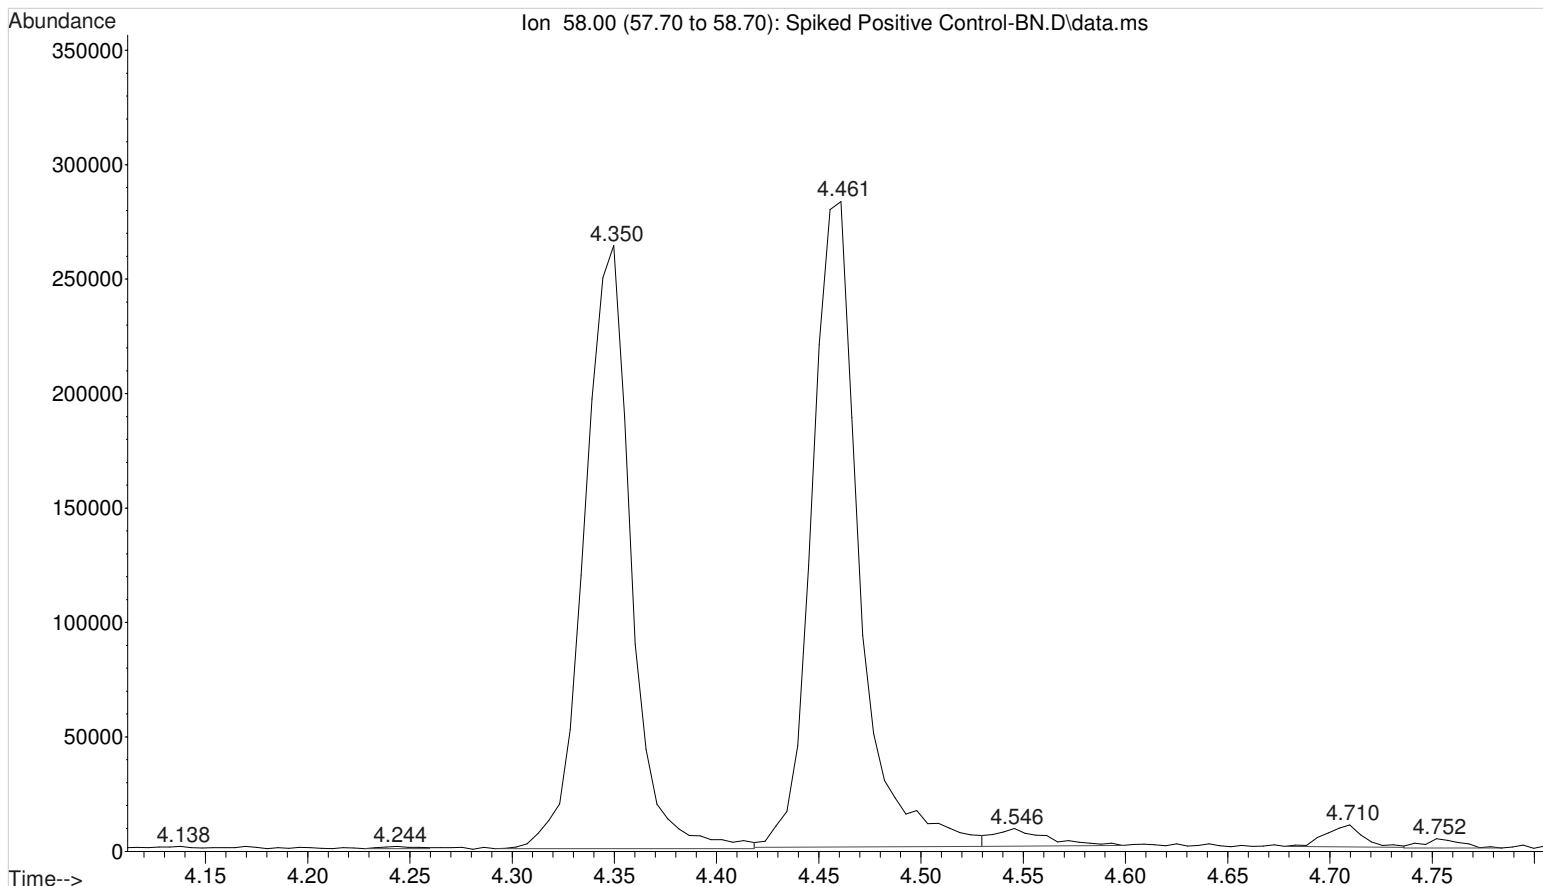



File :F:\10052016\10052016\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 05 Oct 2016 12:13 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

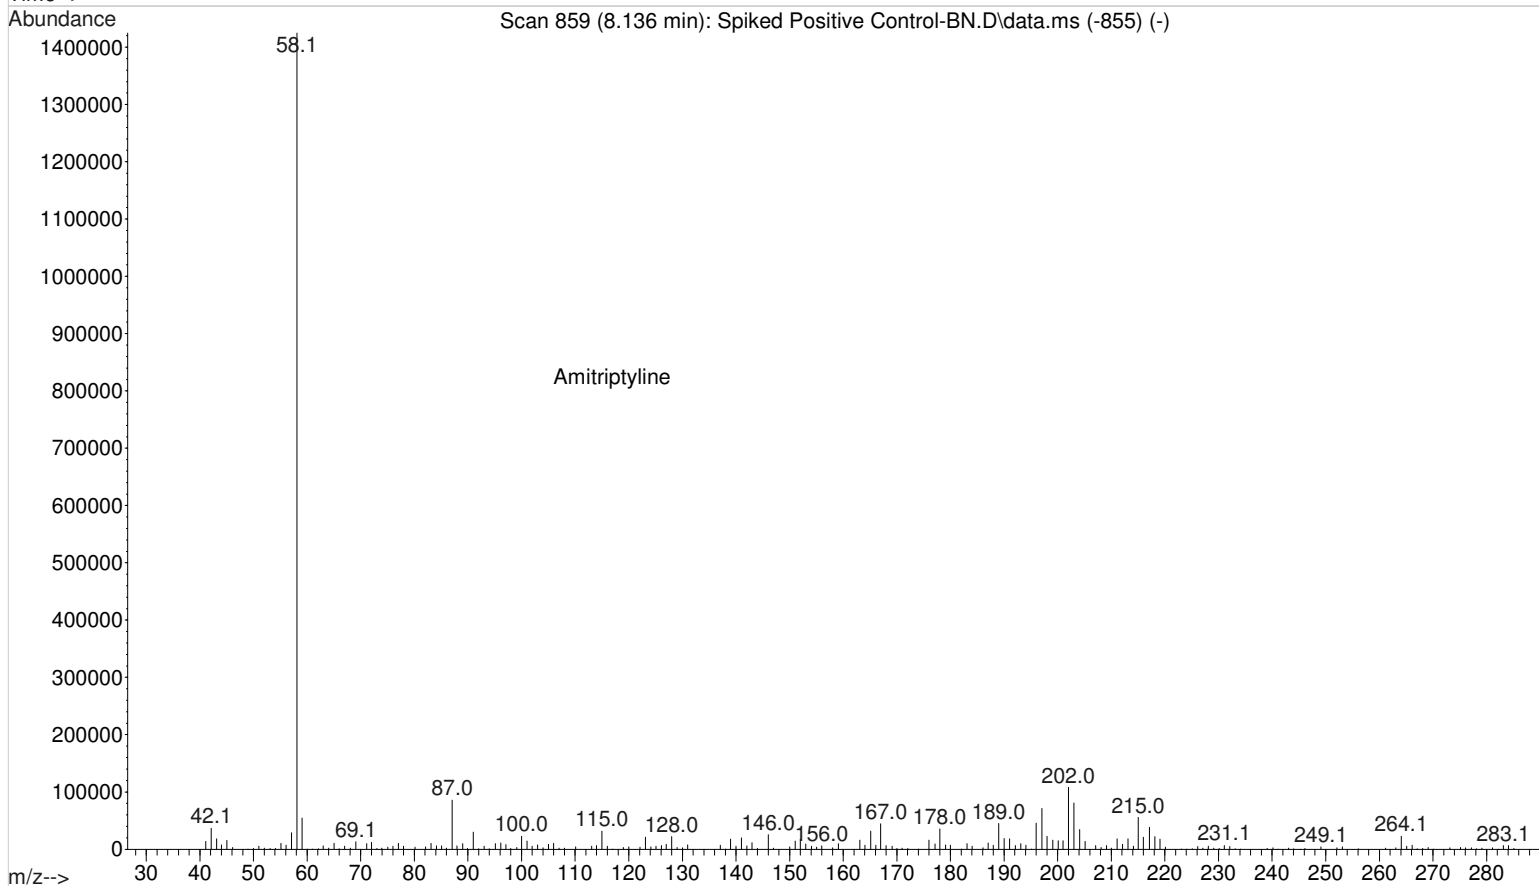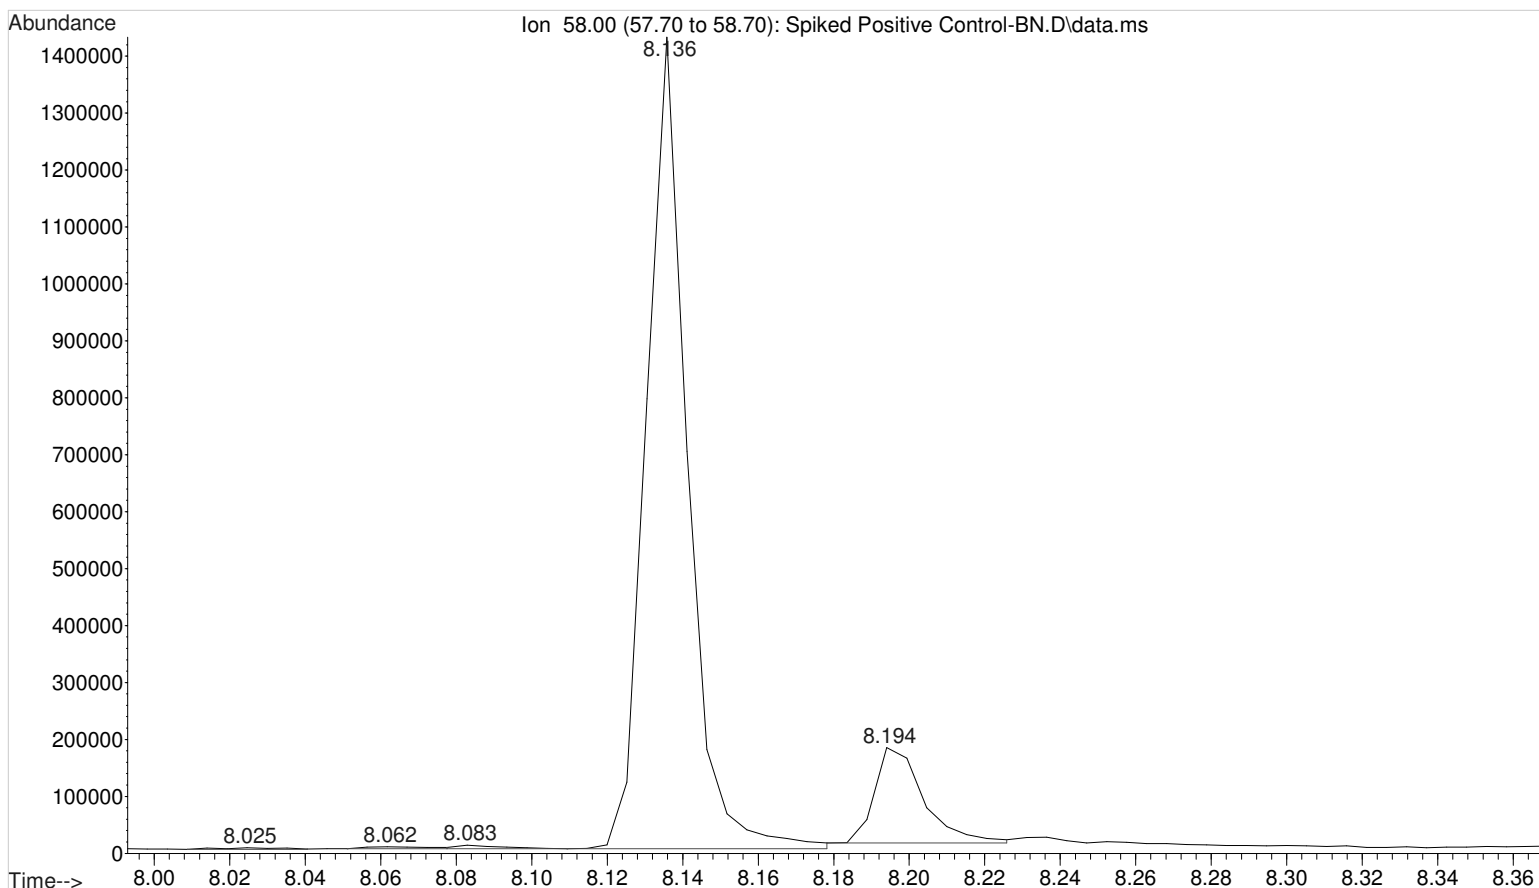


File : F:\10052016\10052016\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 05 Oct 2016 12:13 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name : Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

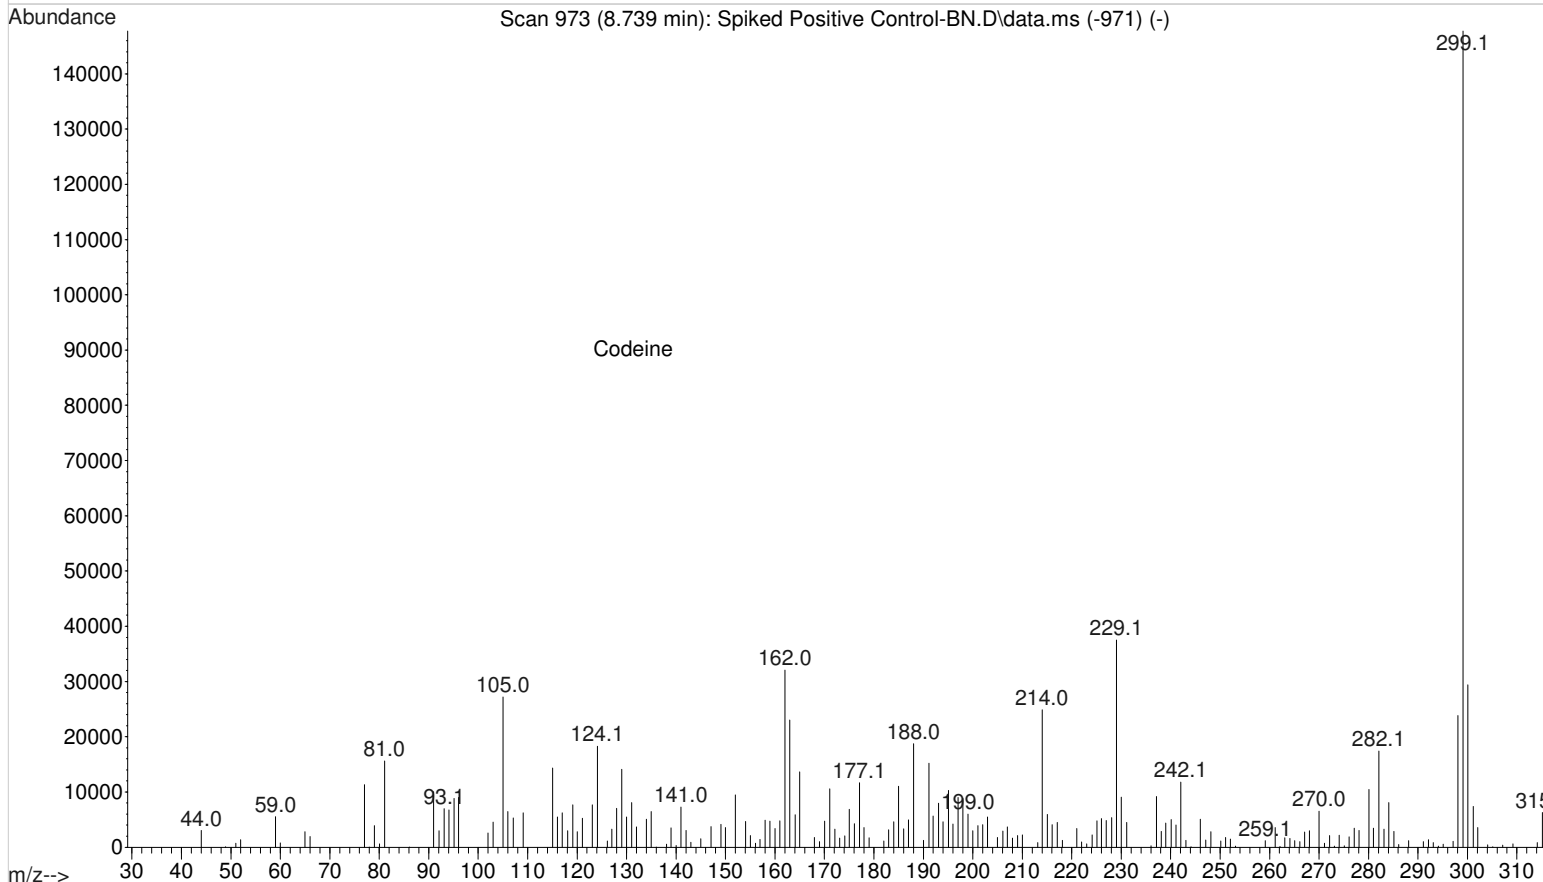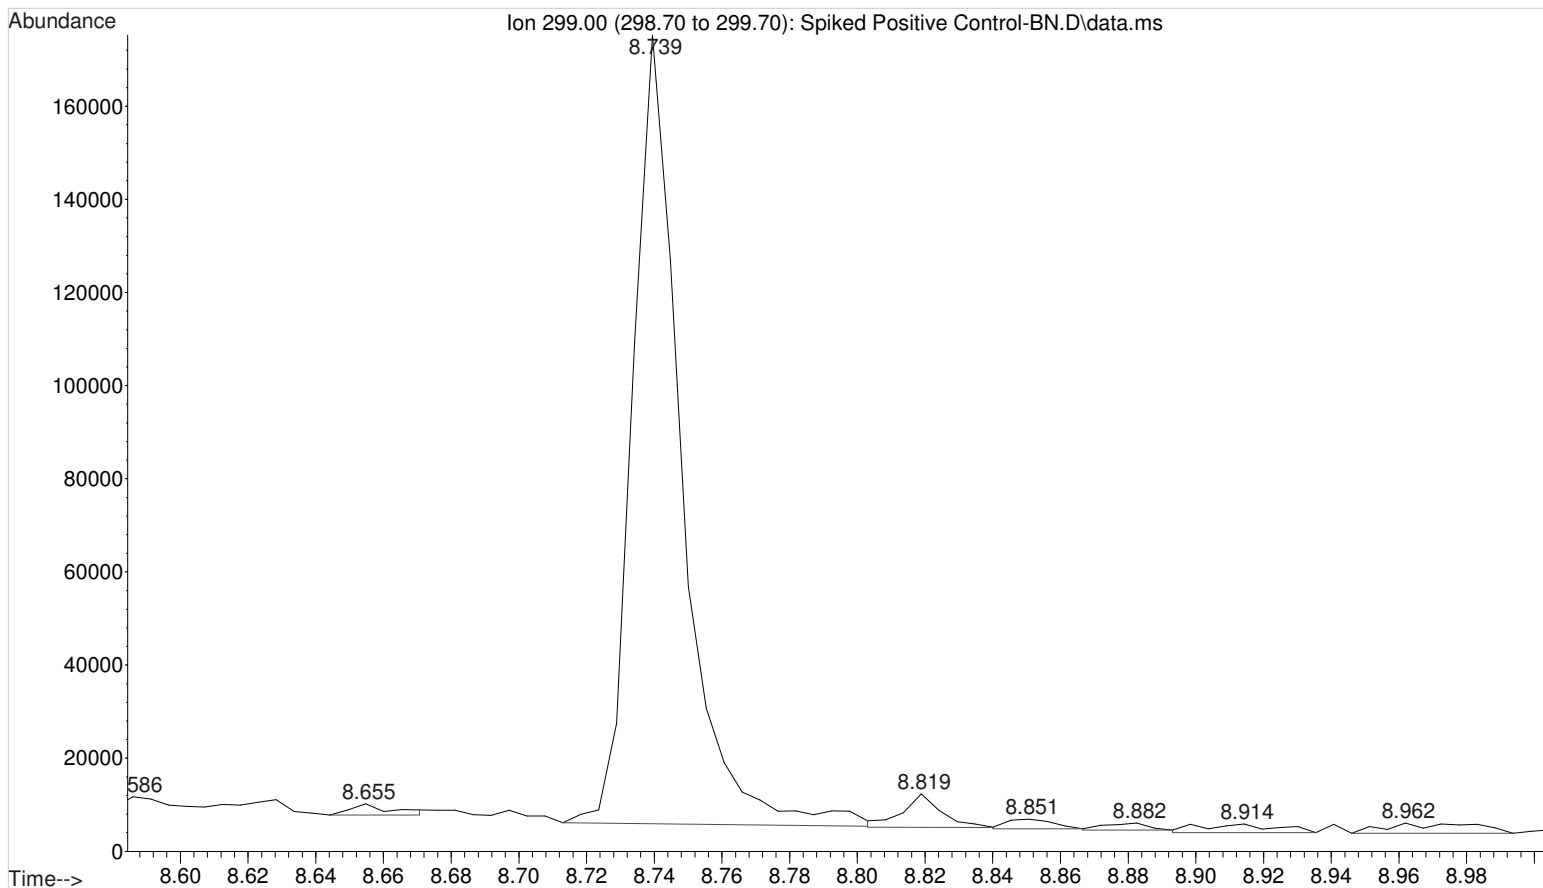


File : F:\10052016\10052016\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 05 Oct 2016 12:13 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name : Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

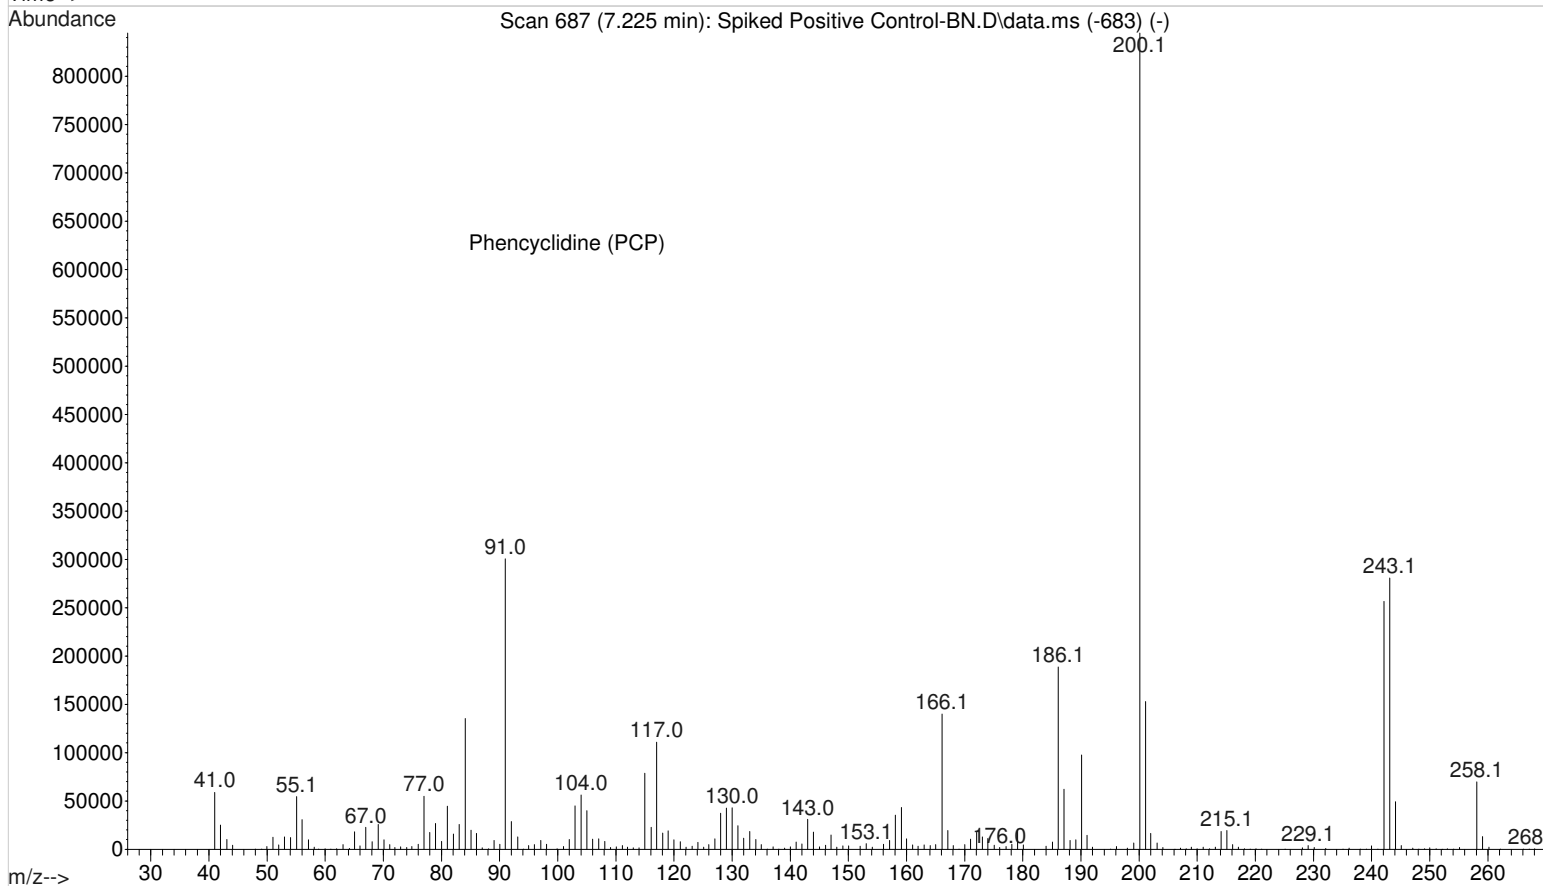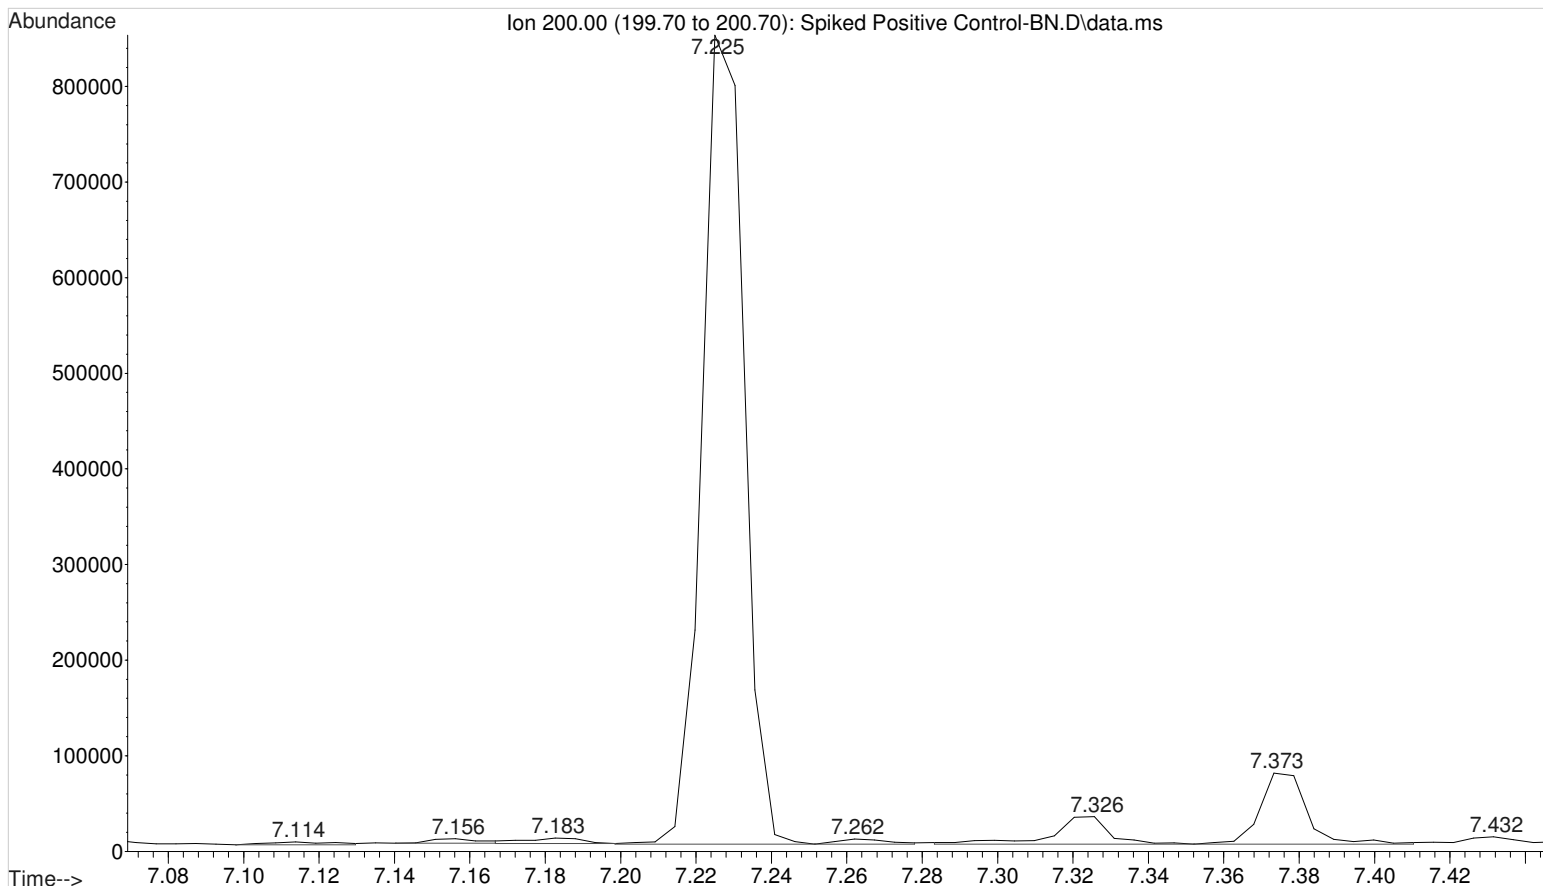


File :F:\10052016\10052016\10052016\Prerun Solvent Blankr.D
Operator : ISP\datastor
Acquired : 05 Oct 2016 12:58 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Pre-run Solvent Blank
Misc Info : Chloroform
Vial Number: 100

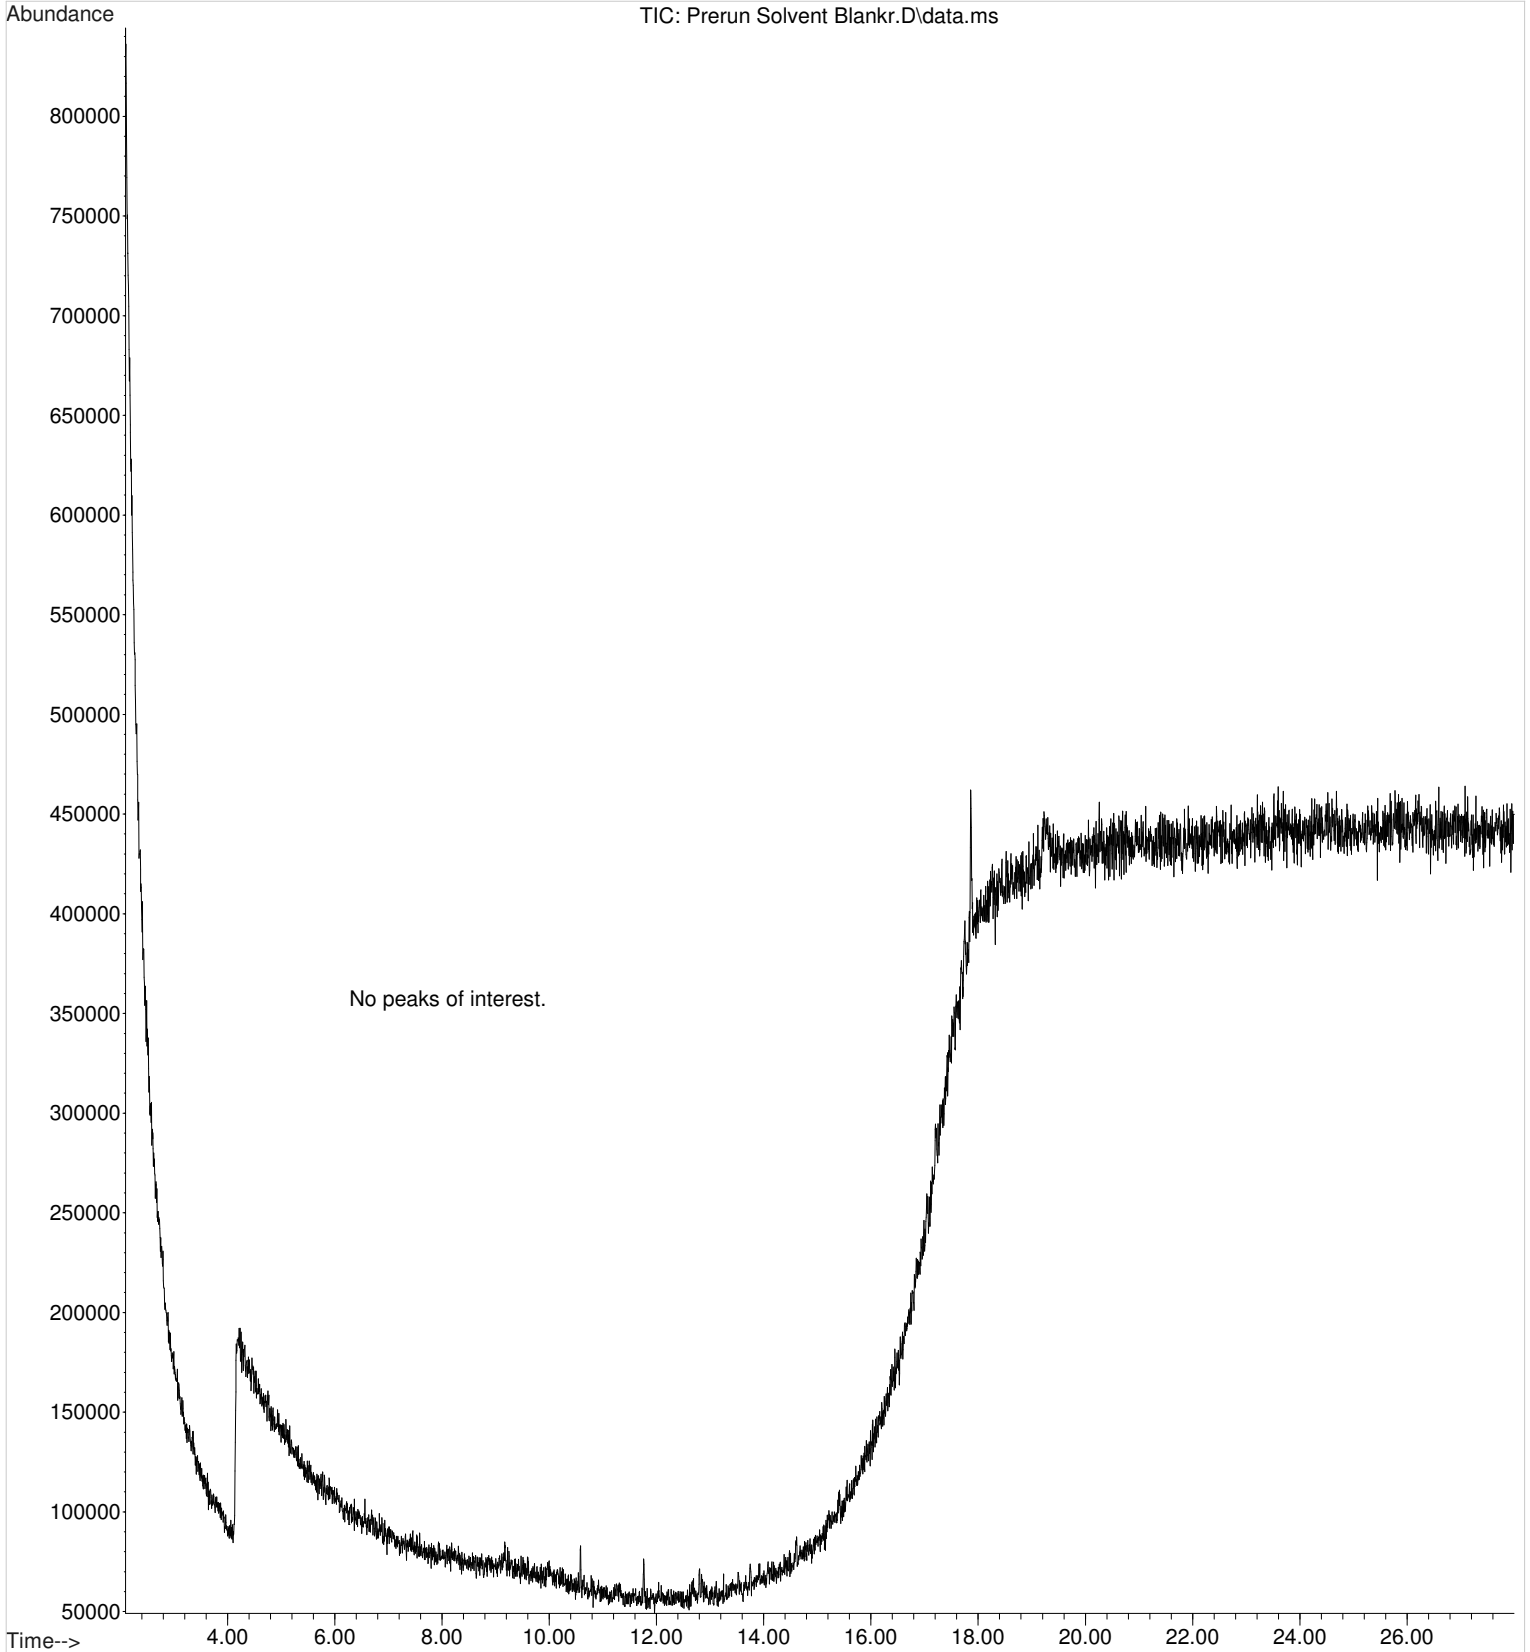



File : F:\10052016\10052016\10052016\prbLK2r.D
Operator : ISP\datastor
Acquired : 05 Oct 2016 14:40 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Solvent Blank
Misc Info : Chloroform
Vial Number: 99

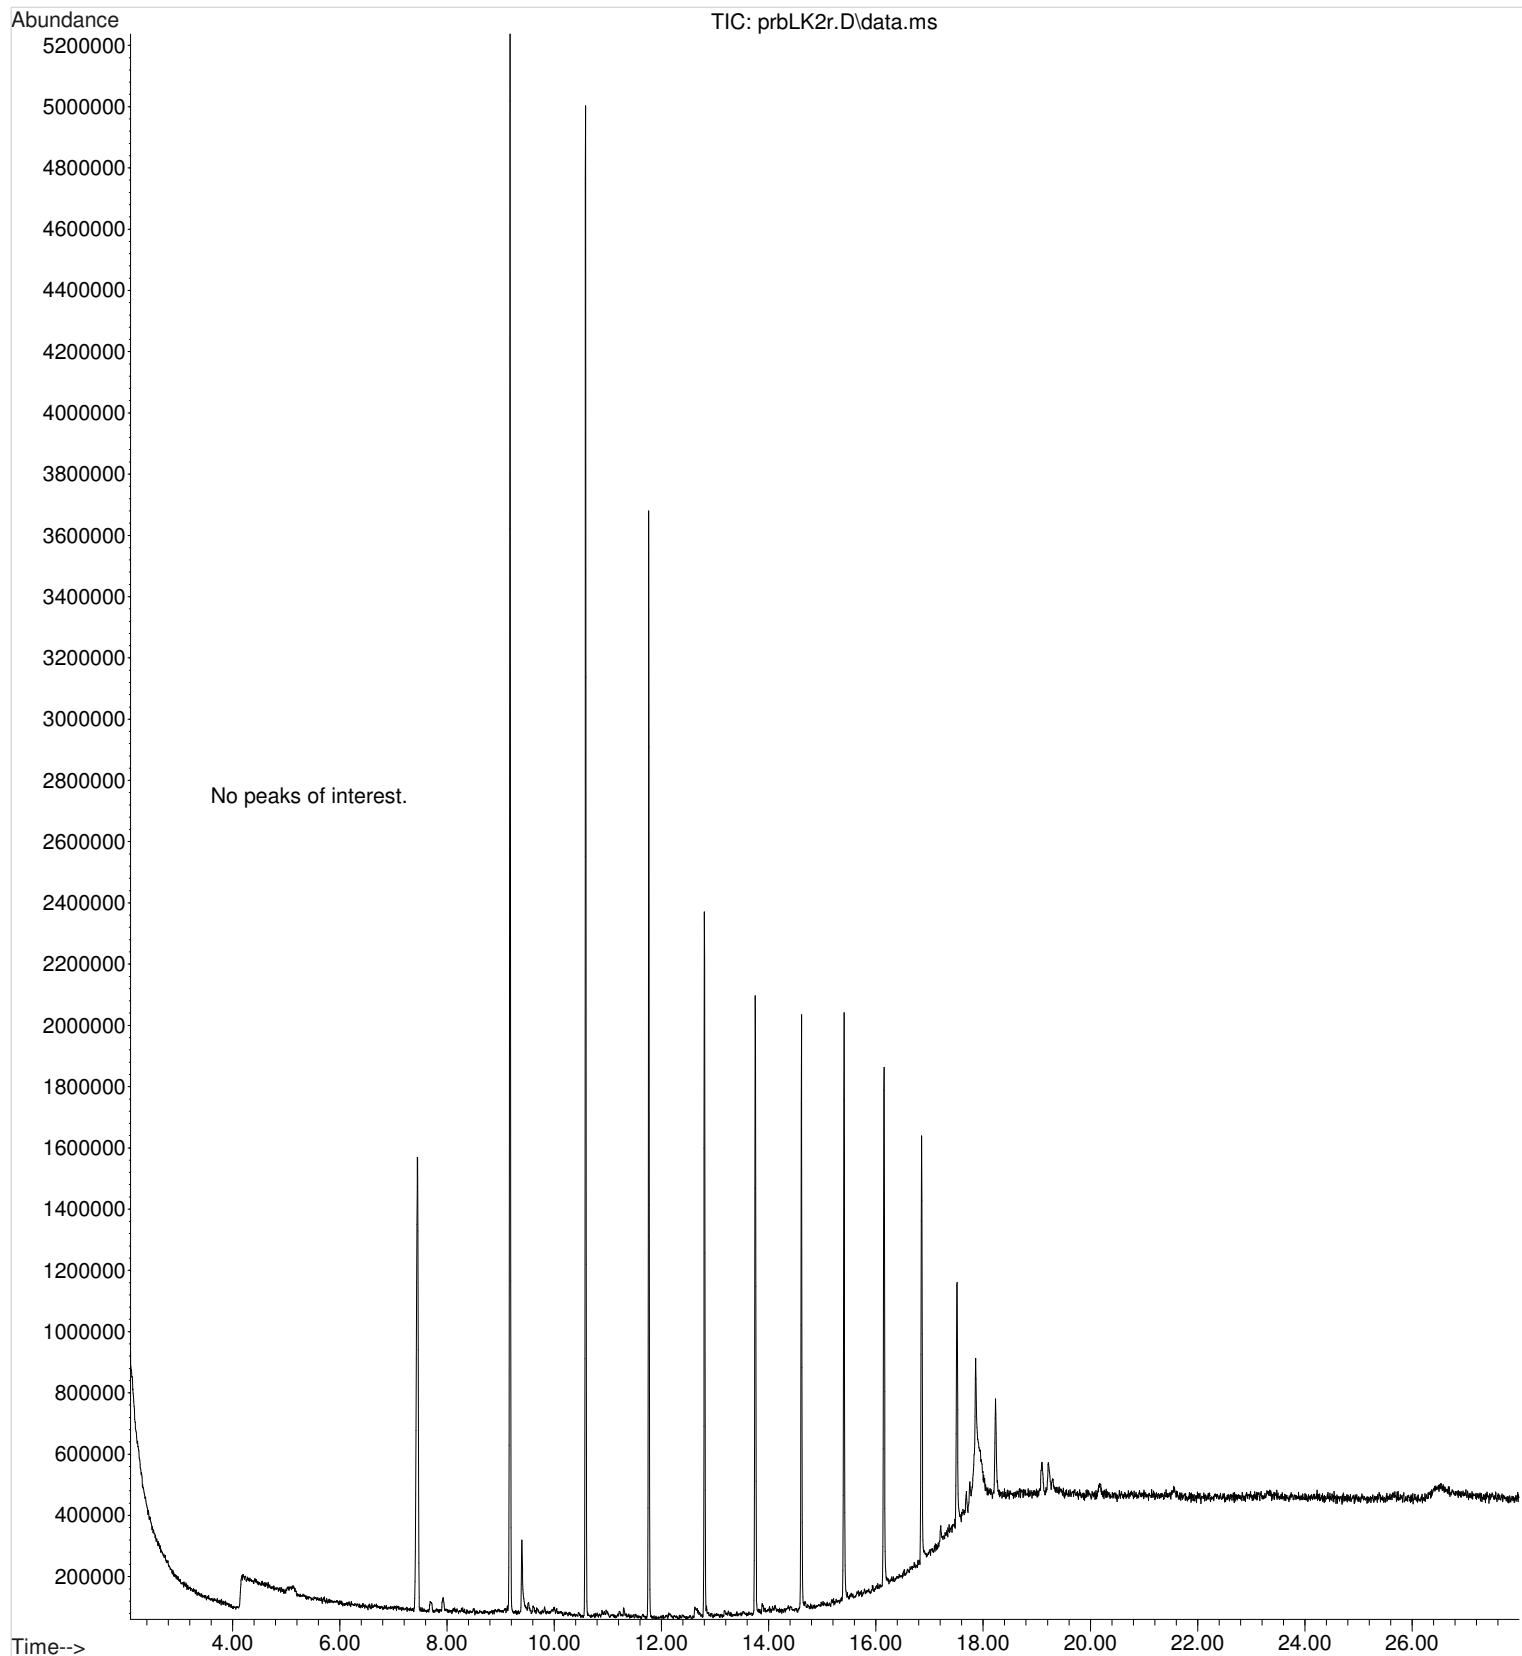



File : F:\10052016\10052016\10052016\Negative Control-BNr.D
Operator : ISP\datastor
Acquired : 05 Oct 2016 13:32 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B1013
Misc Info : Analytical Method 3.6.1
Vial Number: 1

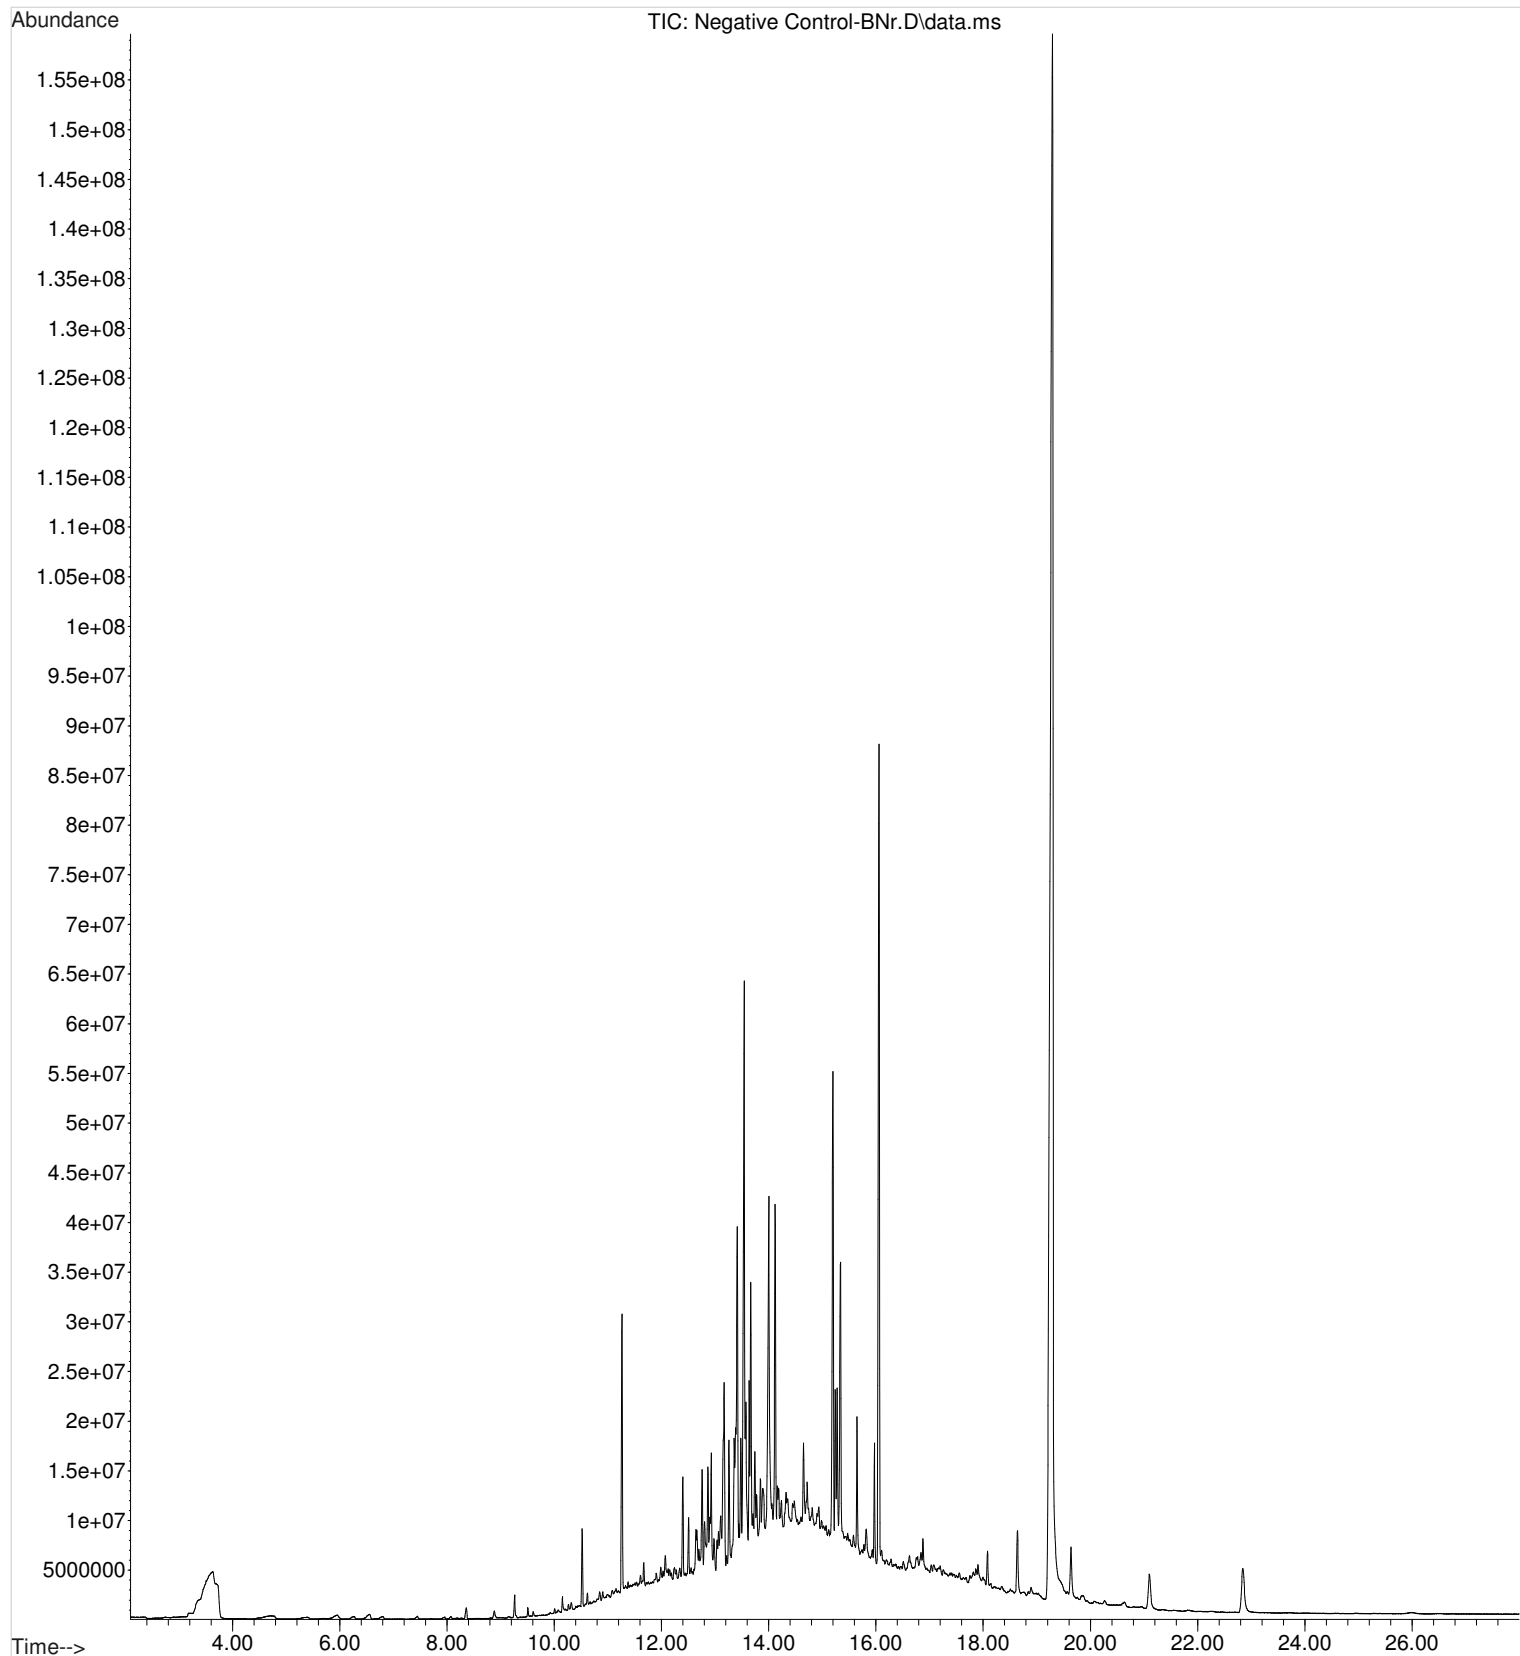


File : F:\10052016\10052016\10052016\Negative Control-BNr.D
Operator : ISP\datastor
Acquired : 05 Oct 2016 13:32 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name : Negative Control - Utak Lot B1013
Misc Info : Analytical Method 3.6.1
Vial Number: 1

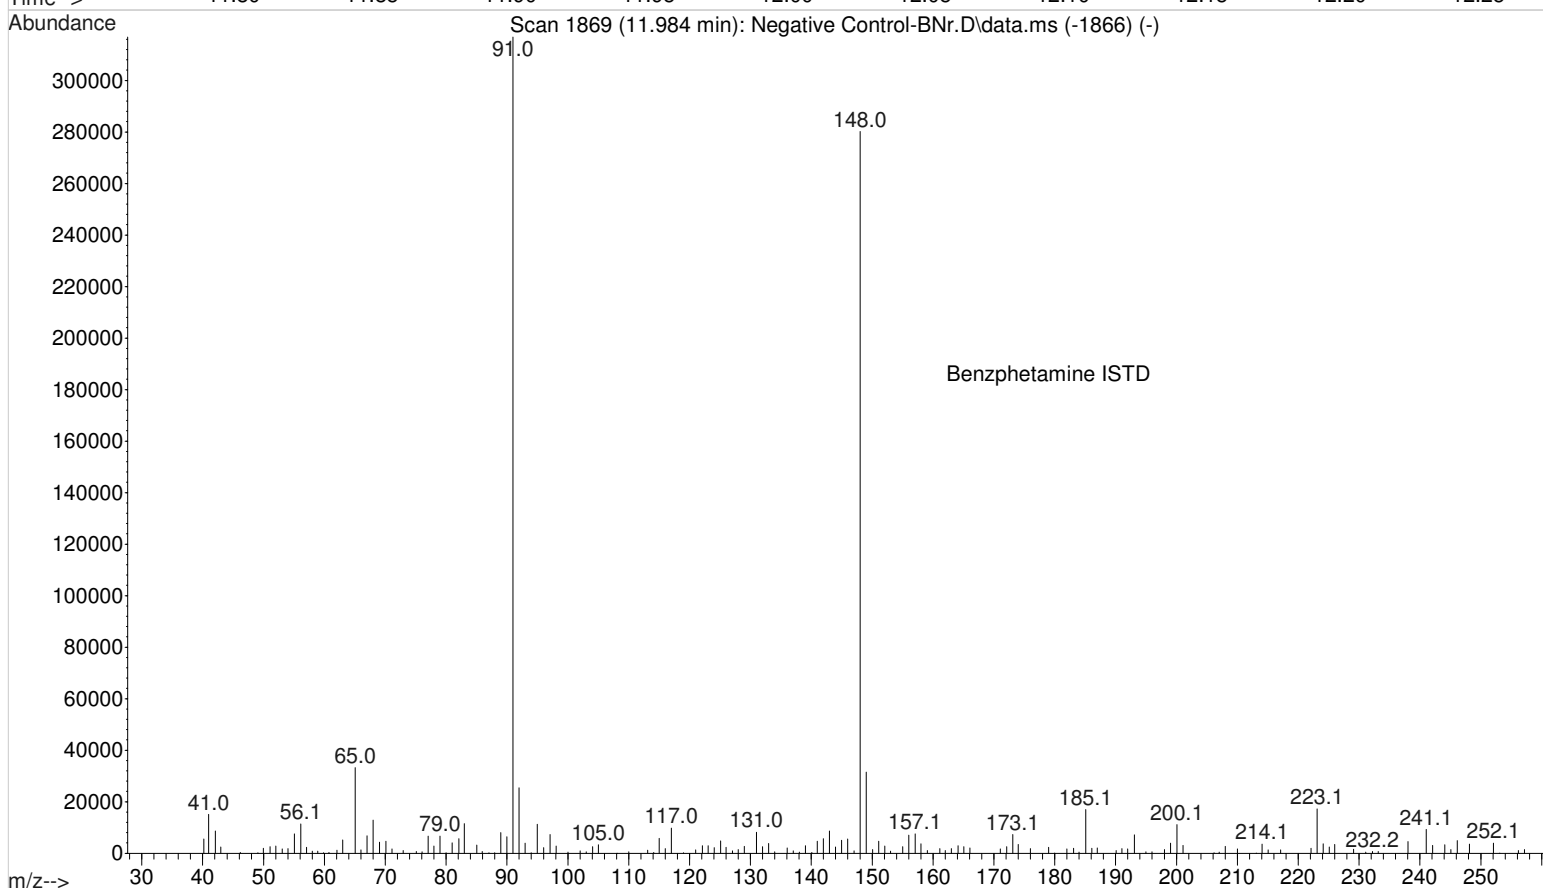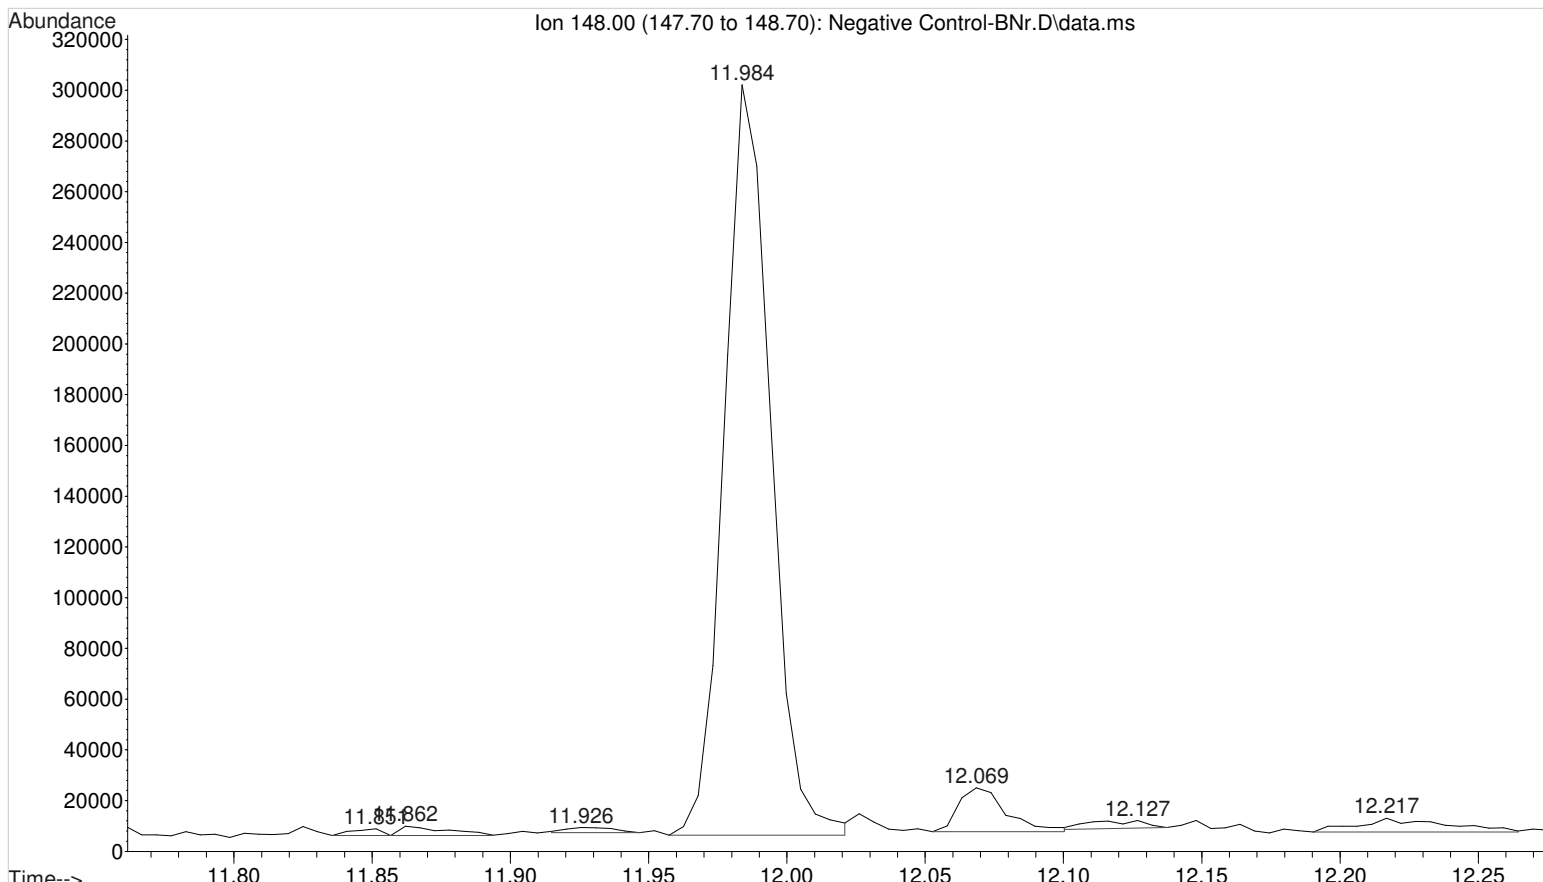



File : F:\10052016\10052016\10052016\Negative Control-BNr.D
Operator : ISP\datastor
Acquired : 05 Oct 2016 13:32 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name : Negative Control - Utak Lot B1013
Misc Info : Analytical Method 3.6.1
Vial Number: 1

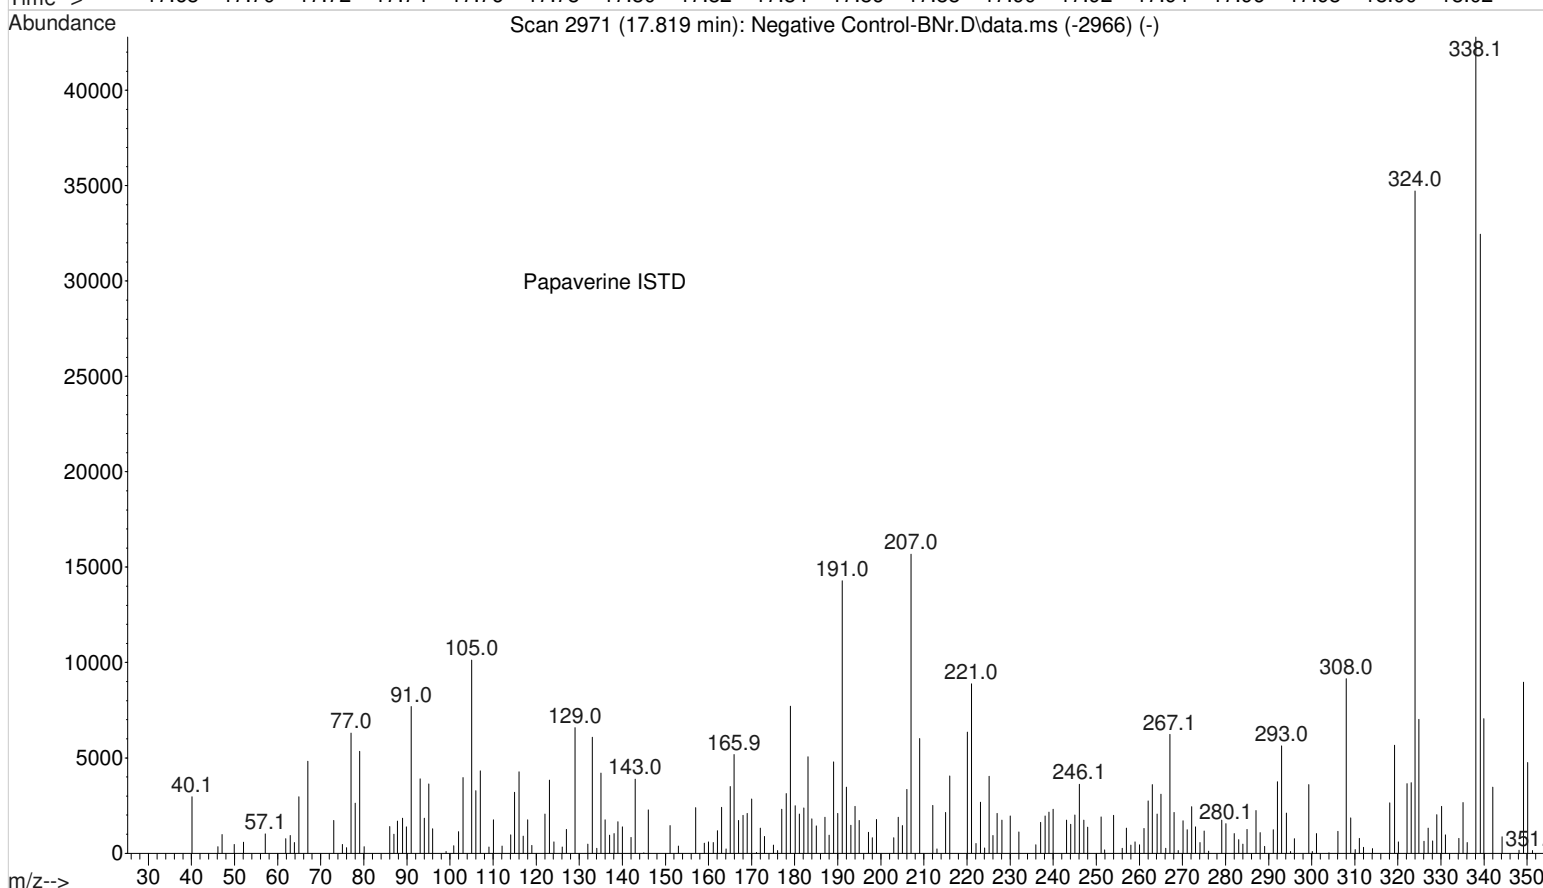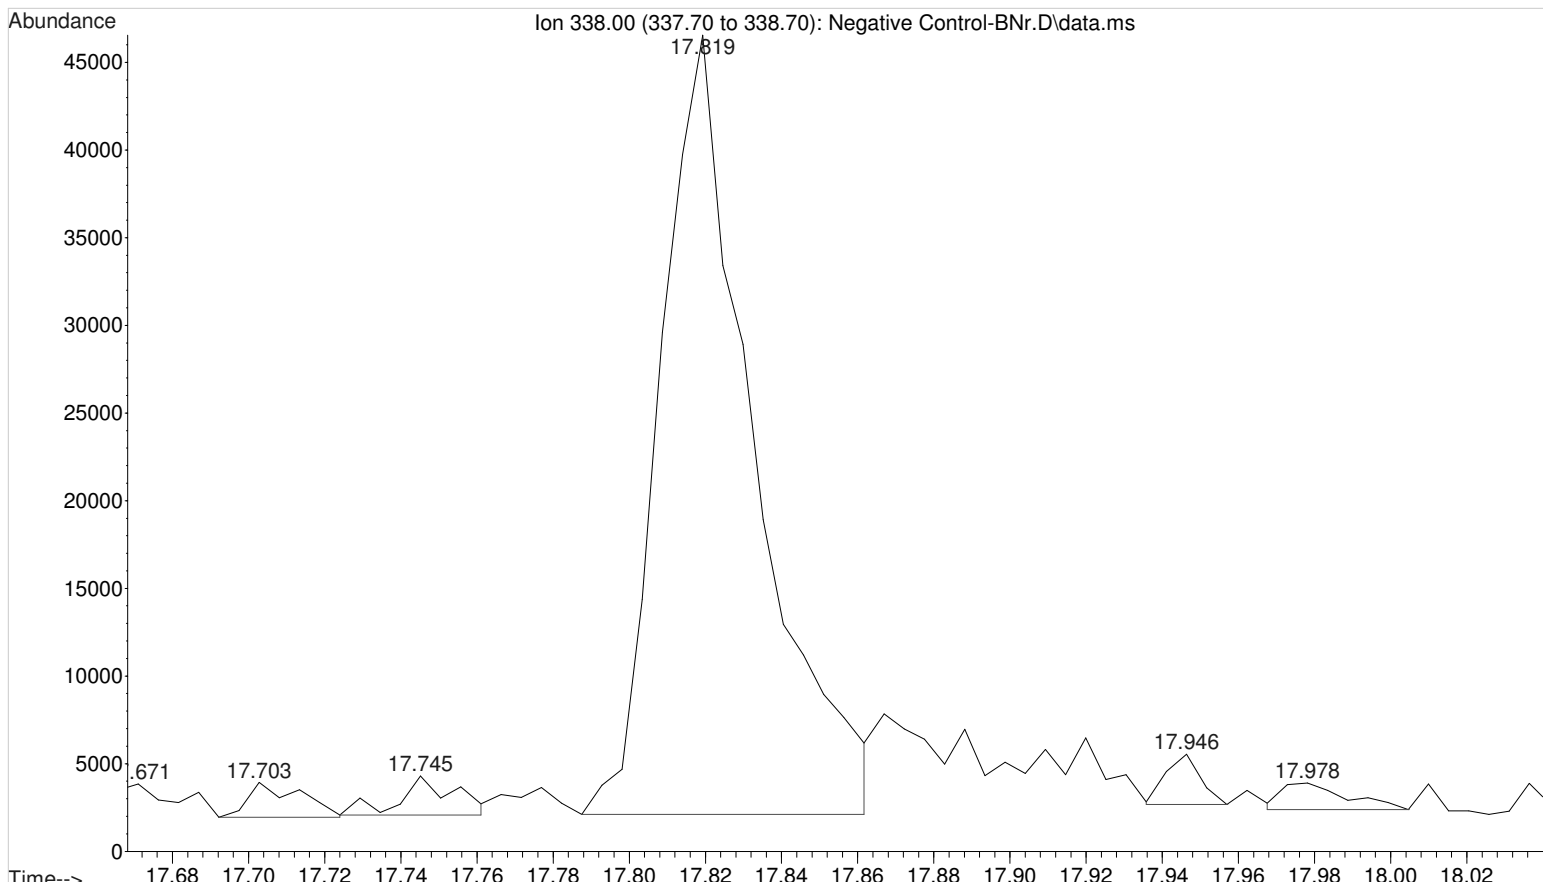



File :F:\10052016\10052016\10052016\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 05 Oct 2016 14:06 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

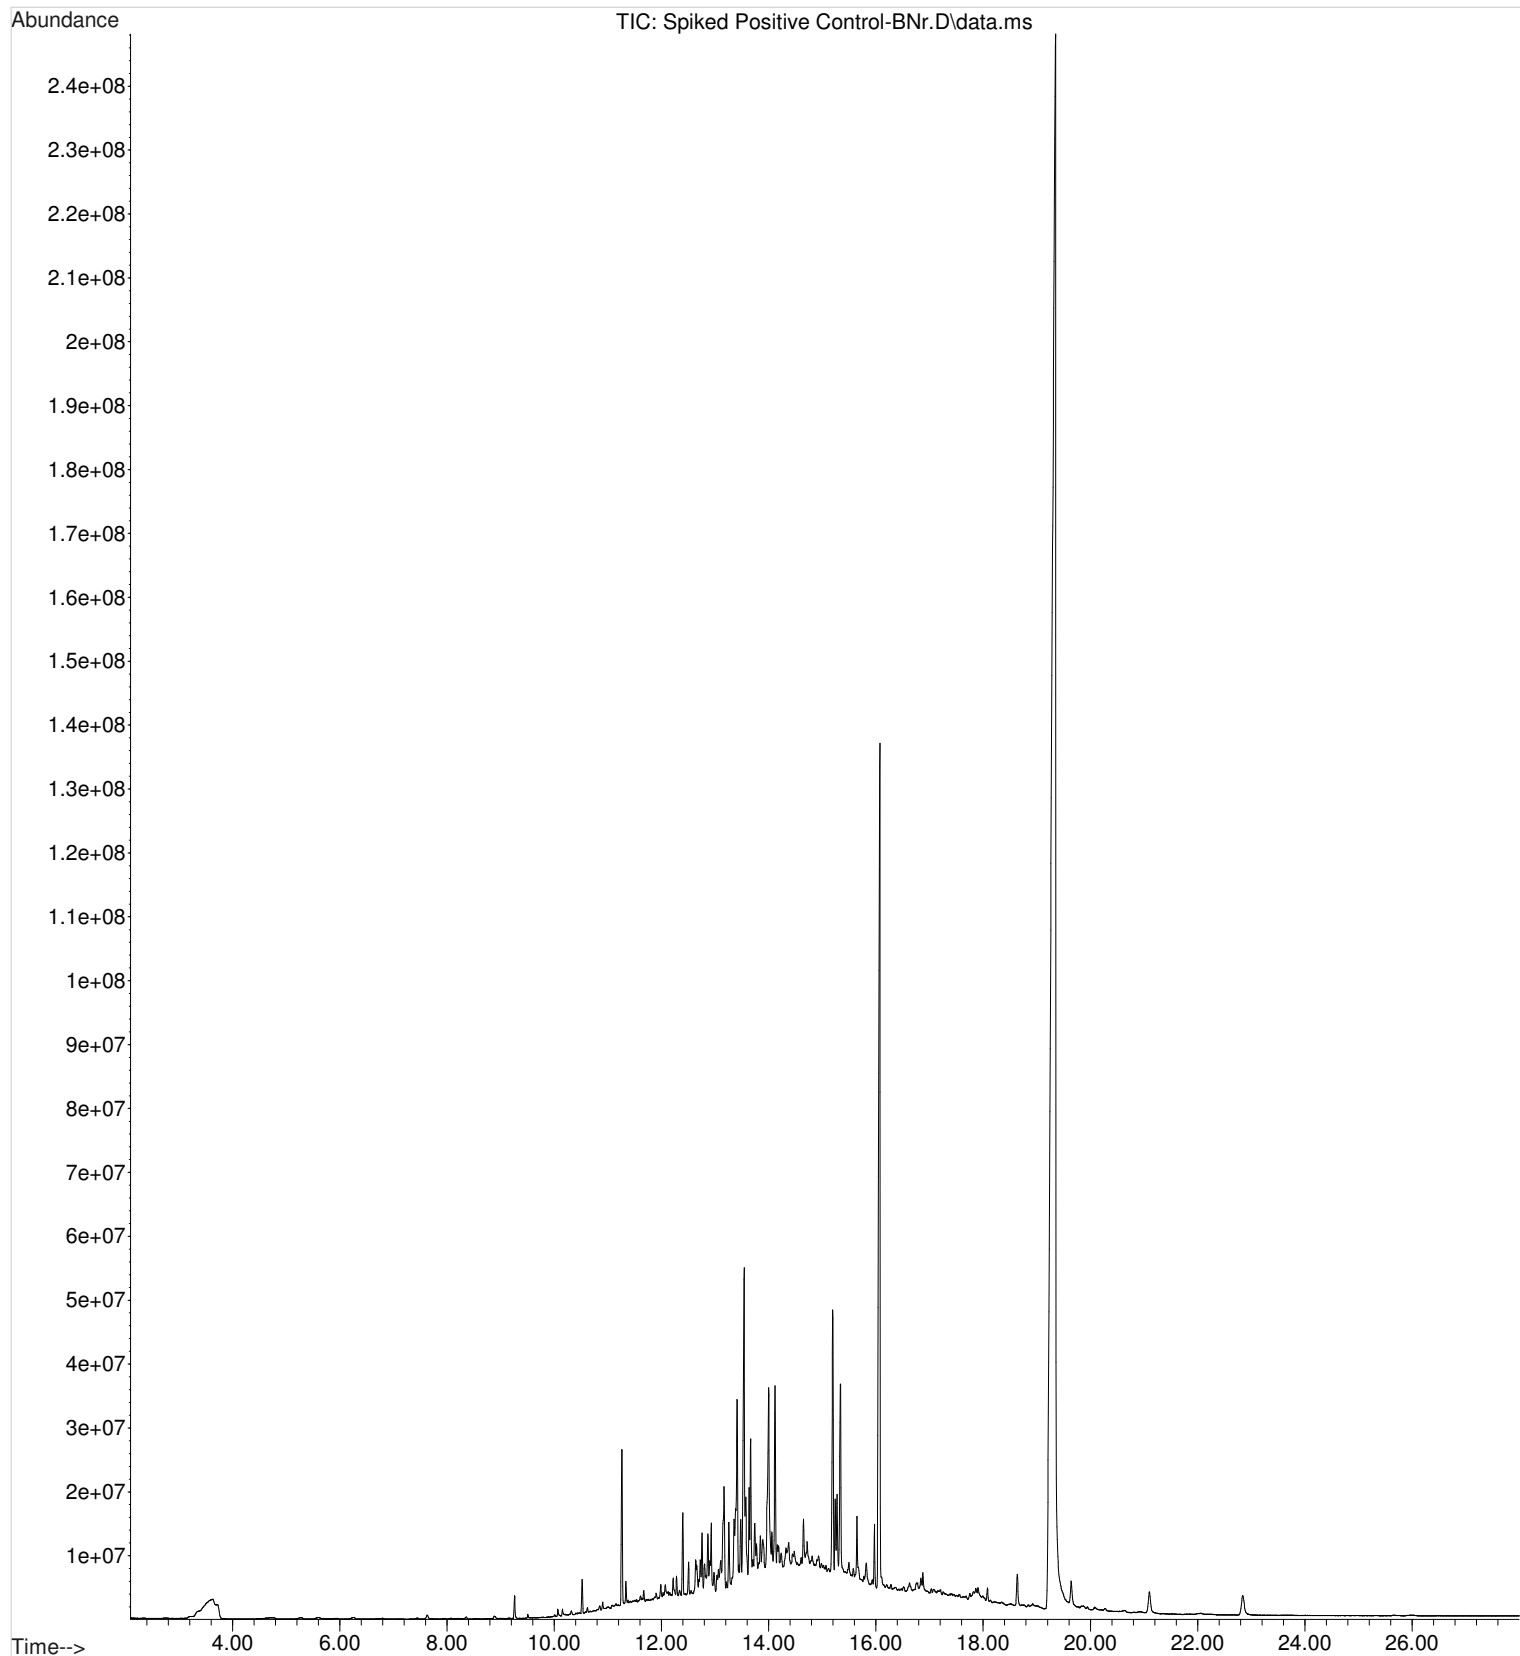



File : F:\10052016\10052016\10052016\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 05 Oct 2016 14:06 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

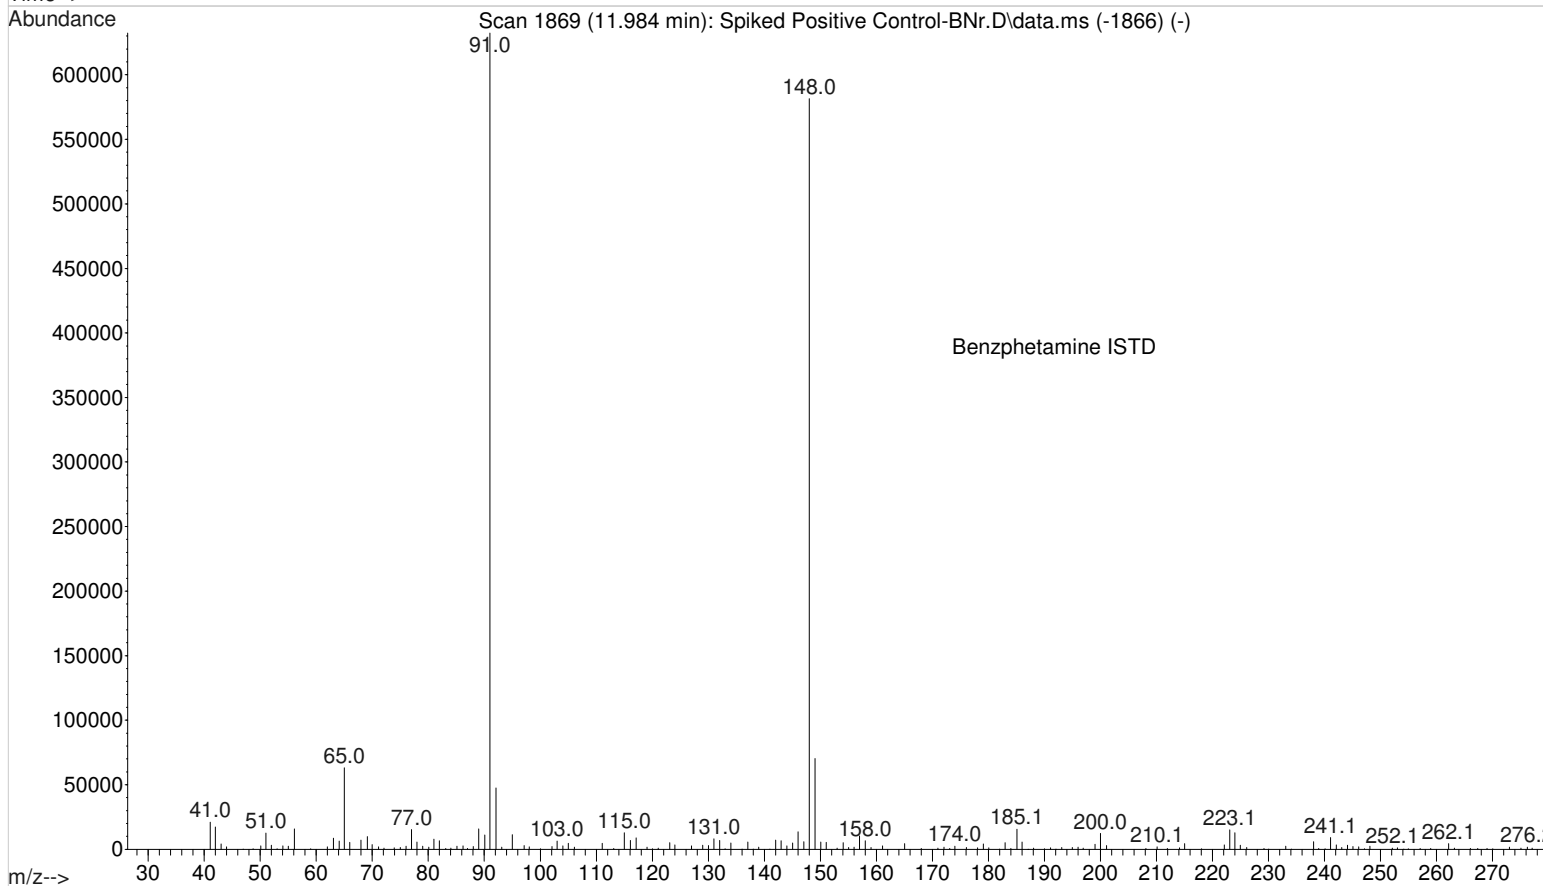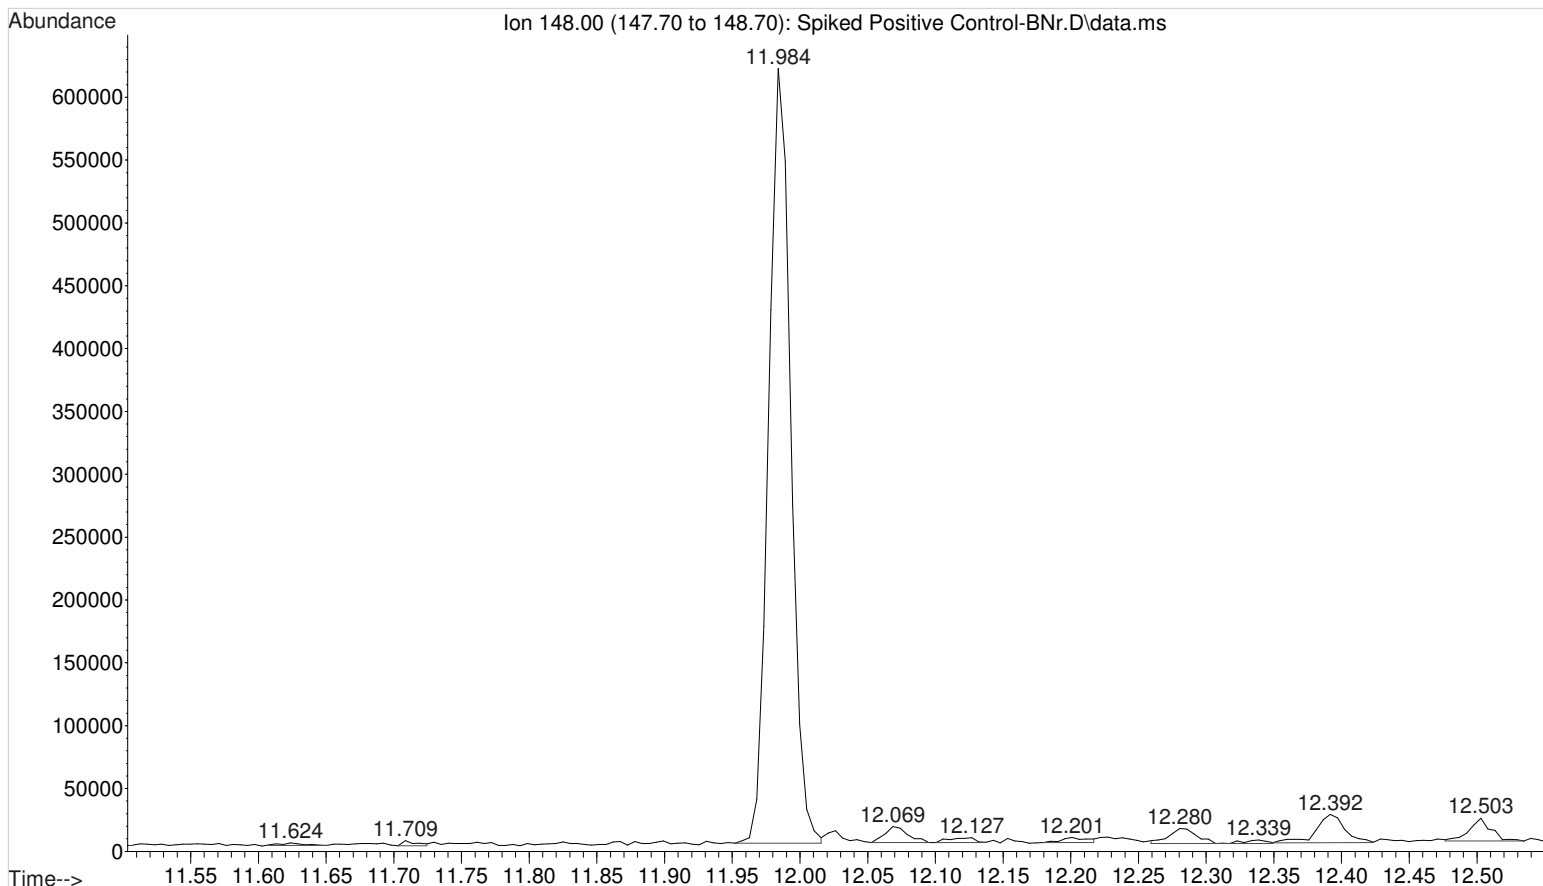



File : F:\10052016\10052016\10052016\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 05 Oct 2016 14:06 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

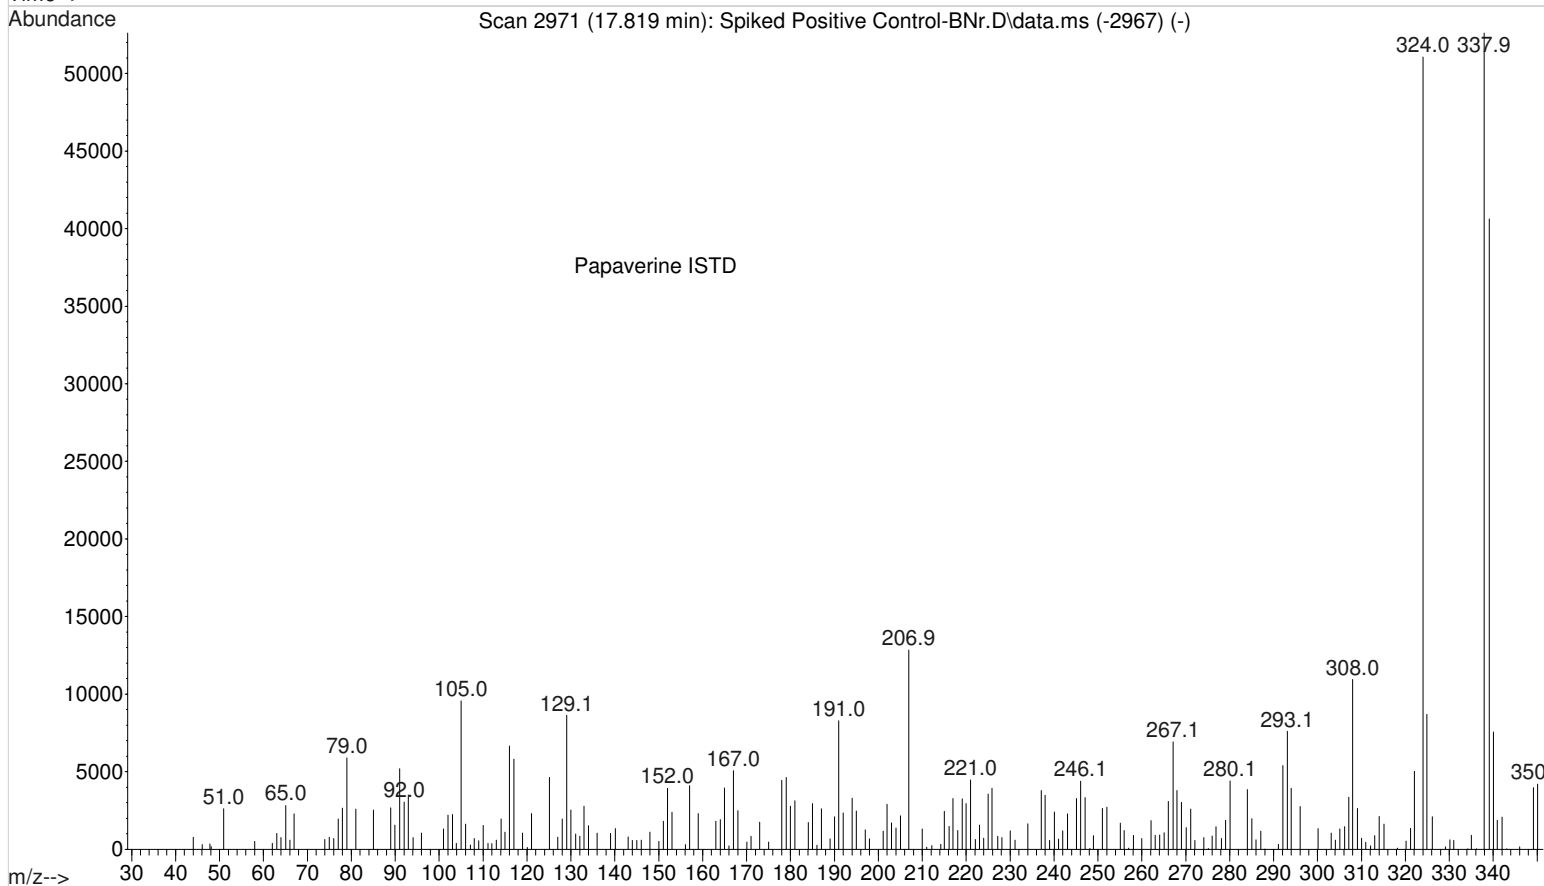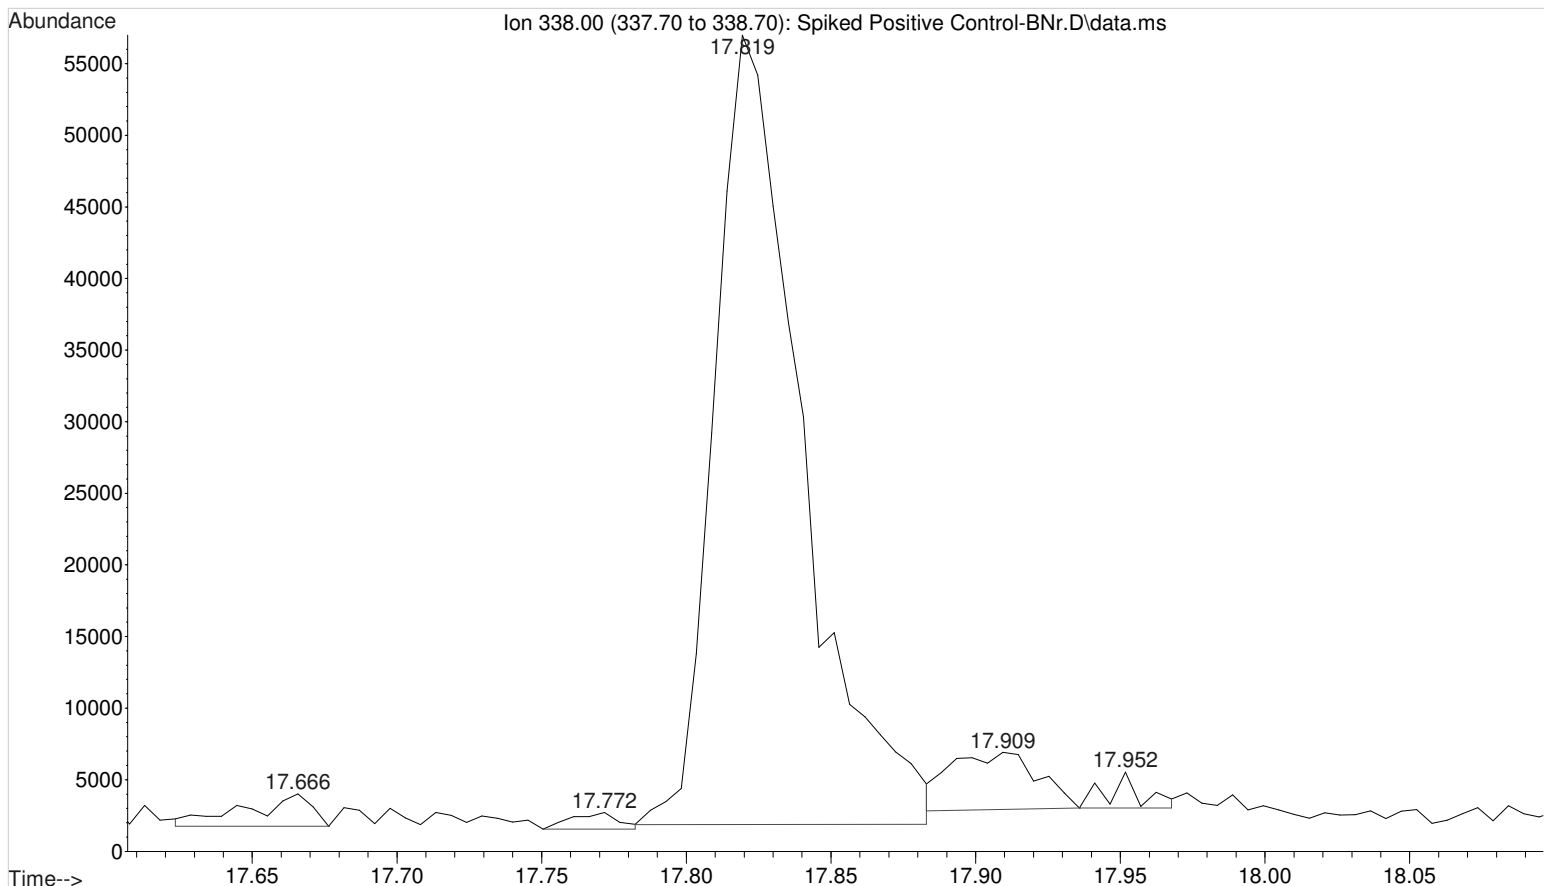



File : F:\10052016\10052016\10052016\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 05 Oct 2016 14:06 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name : Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

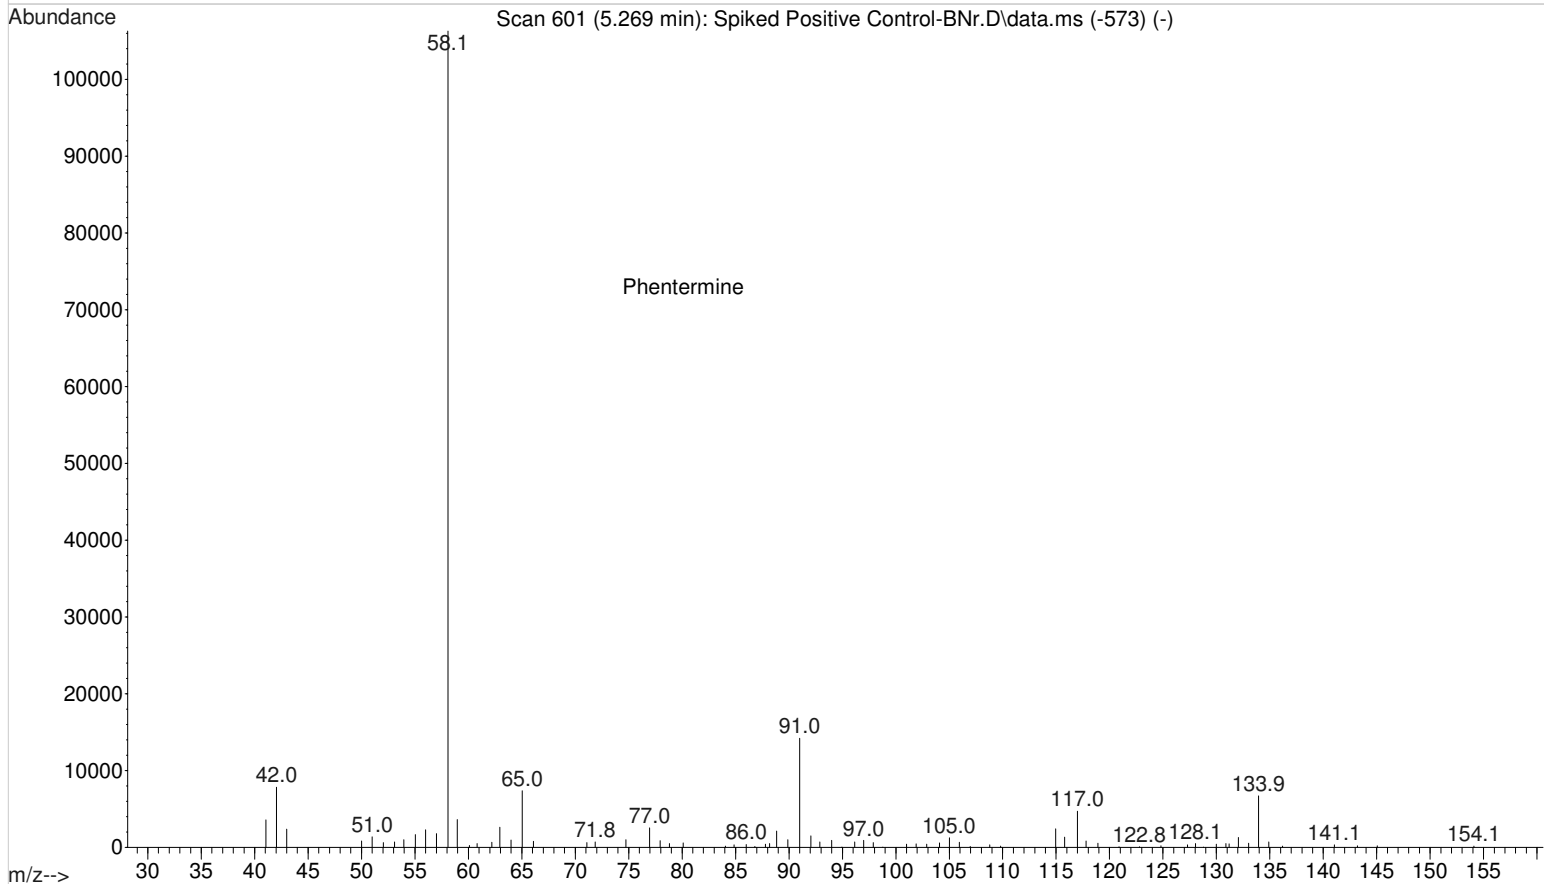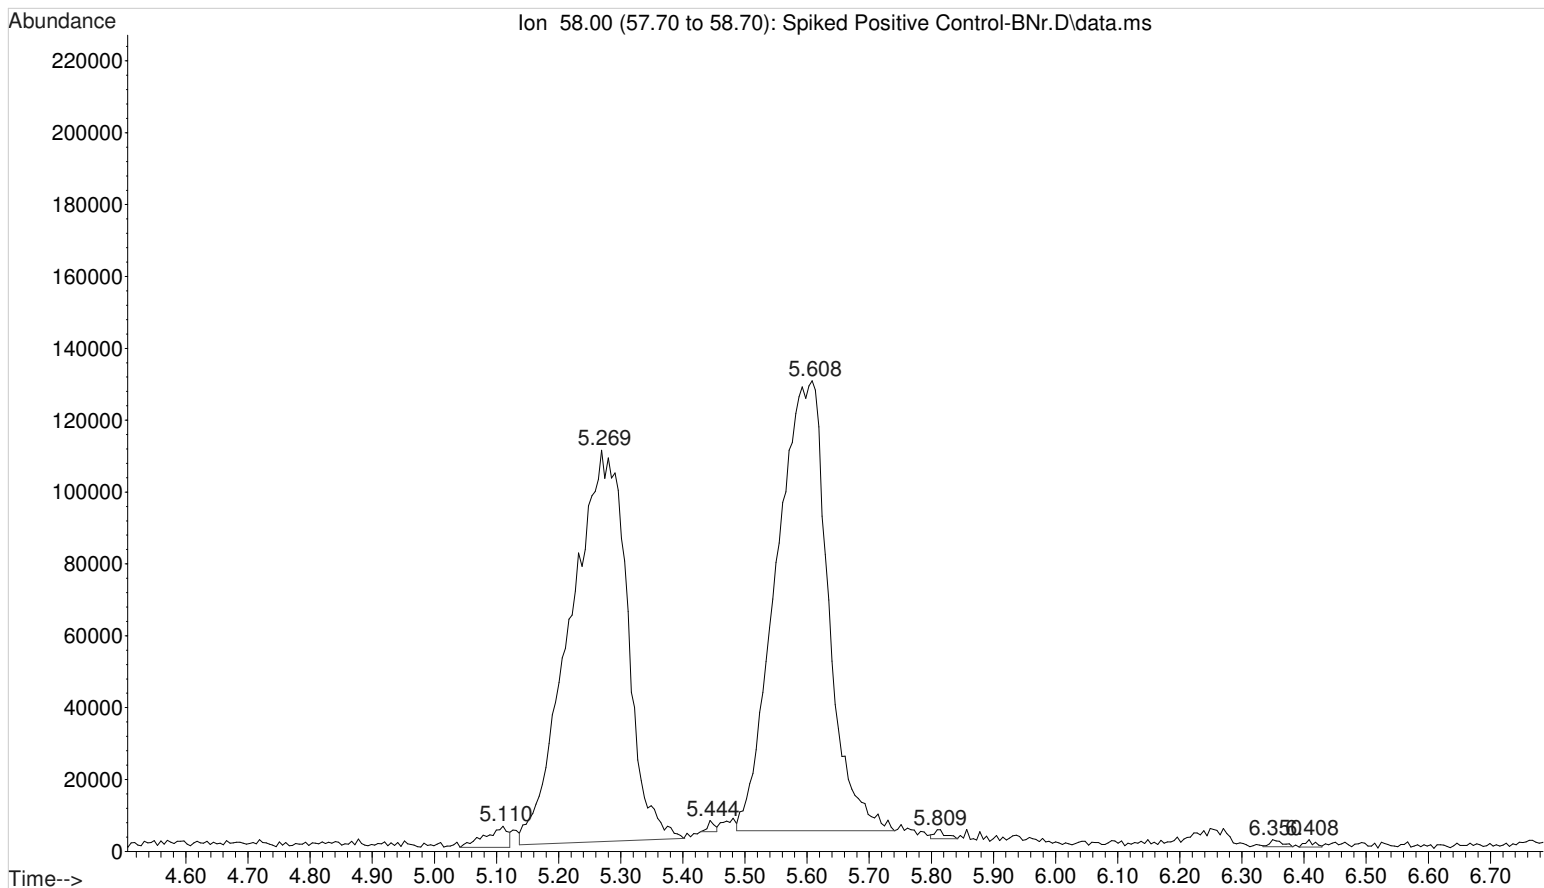



File : F:\10052016\10052016\10052016\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 05 Oct 2016 14:06 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name : Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

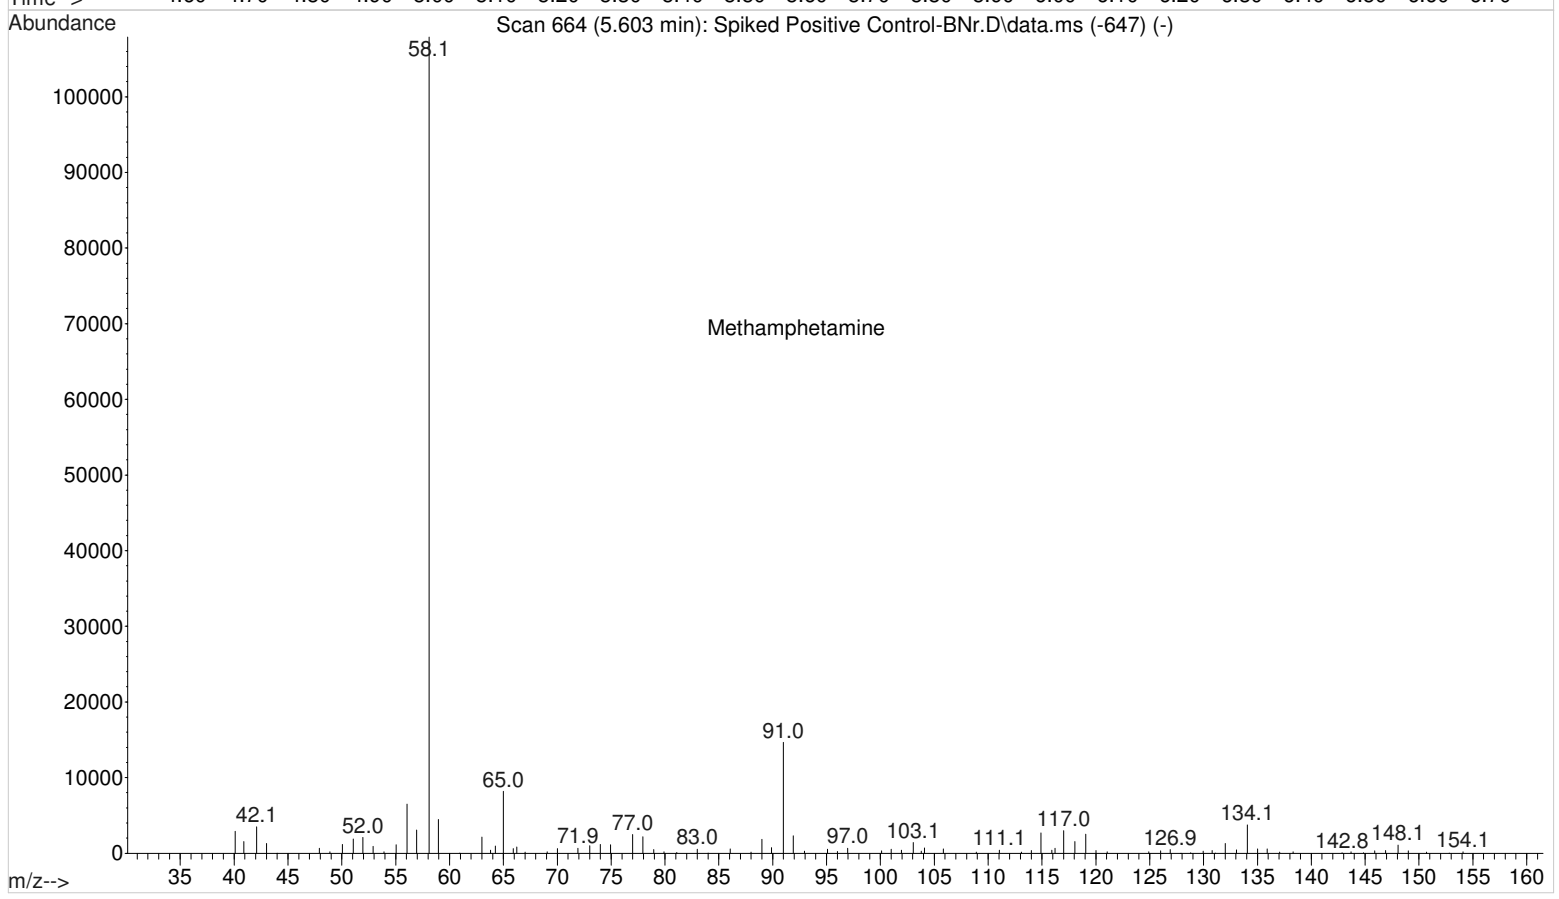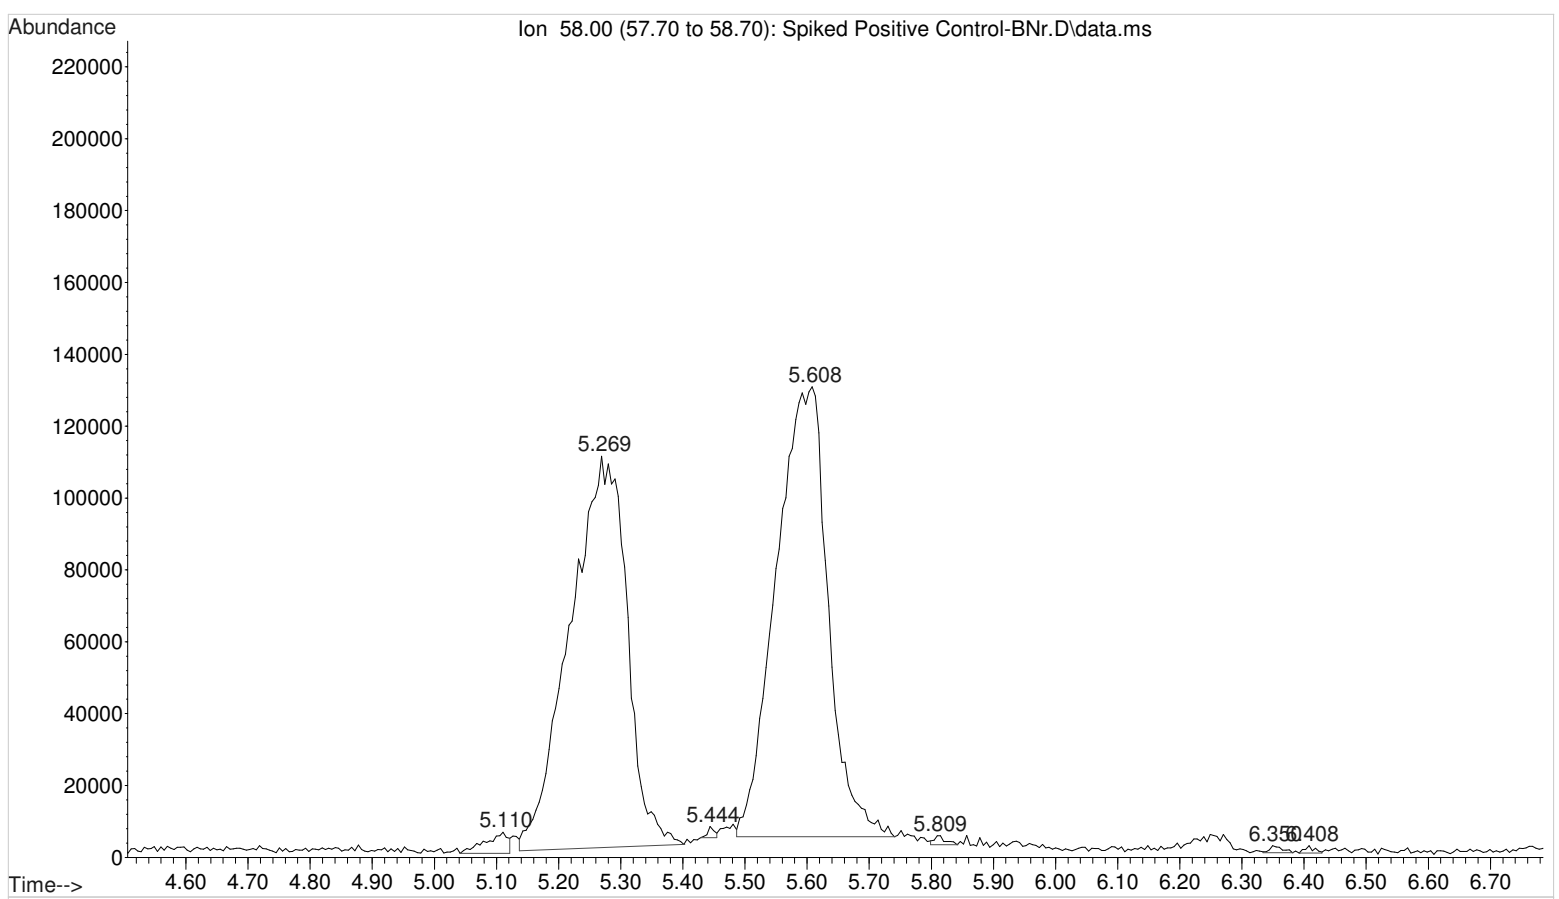

File :F:\10052016\10052016\10052016\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 05 Oct 2016 14:06 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

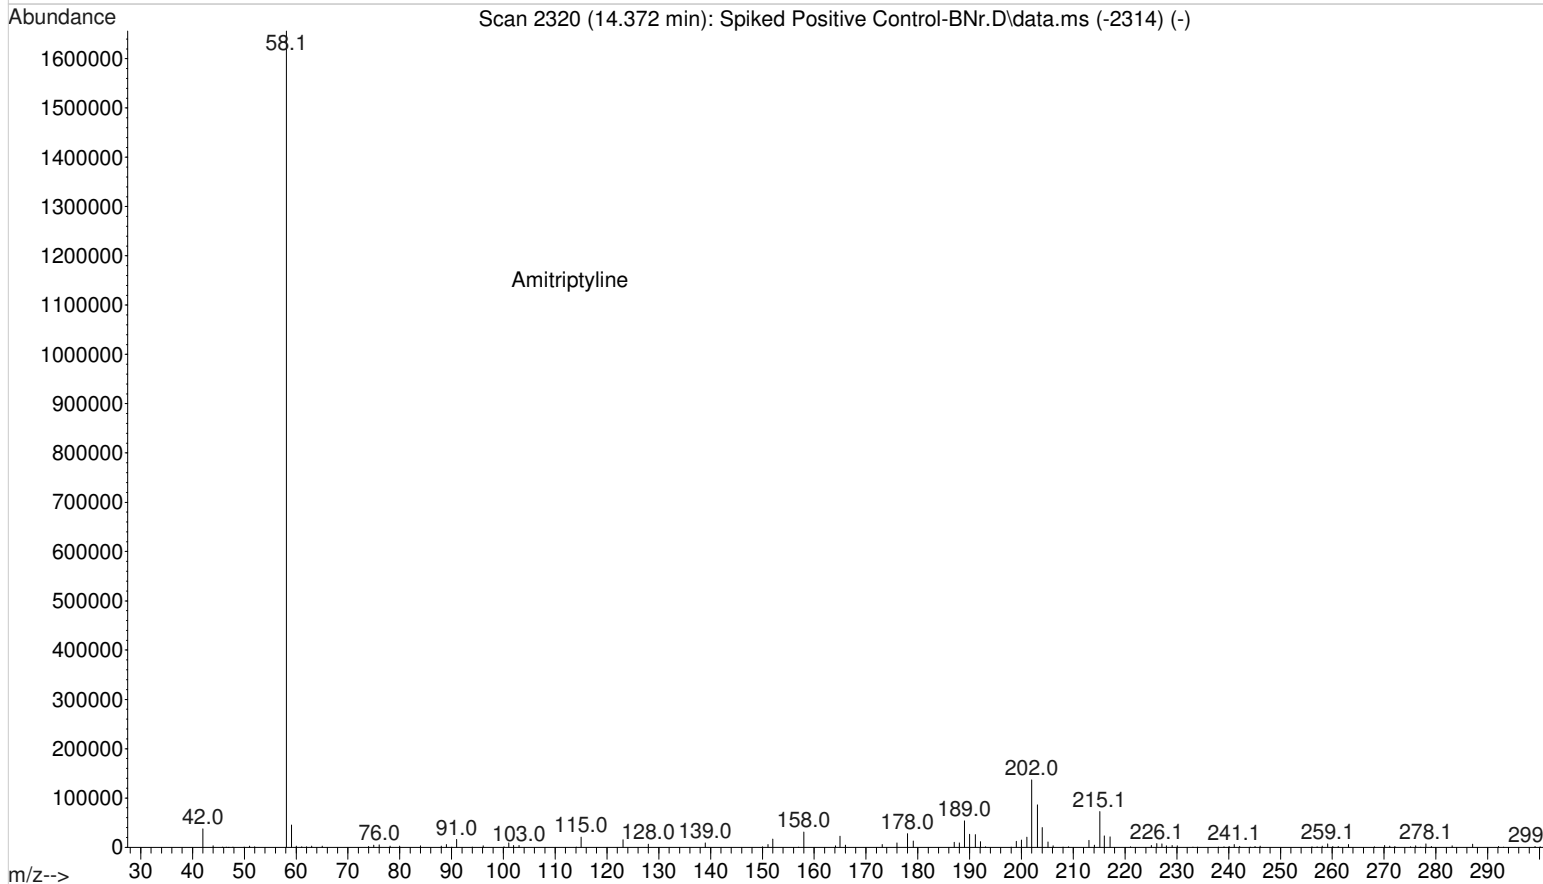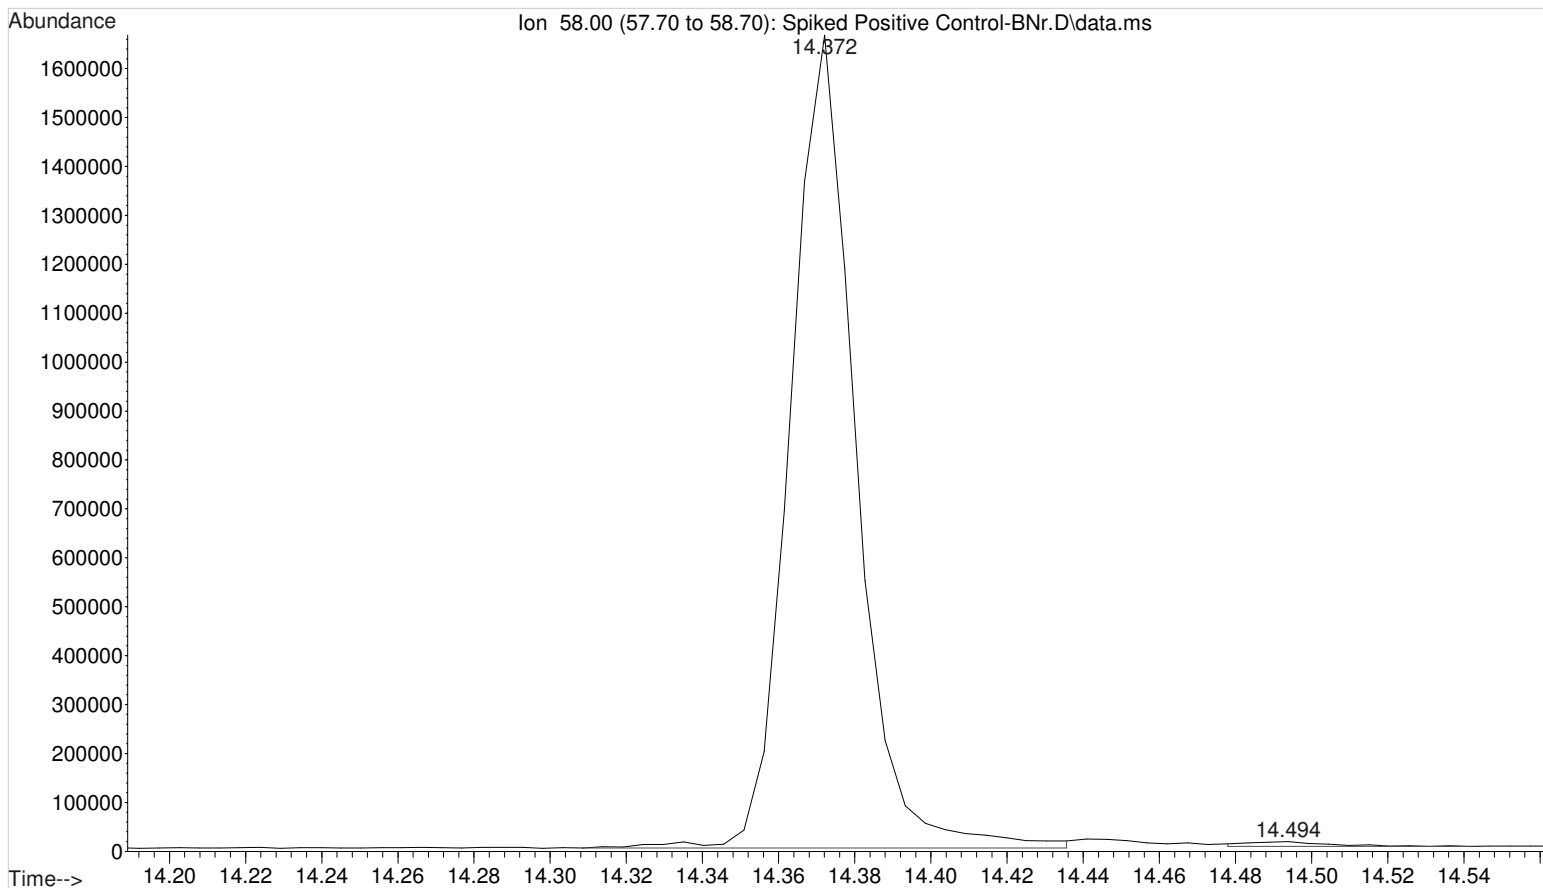

File : F:\10052016\10052016\10052016\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 05 Oct 2016 14:06 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

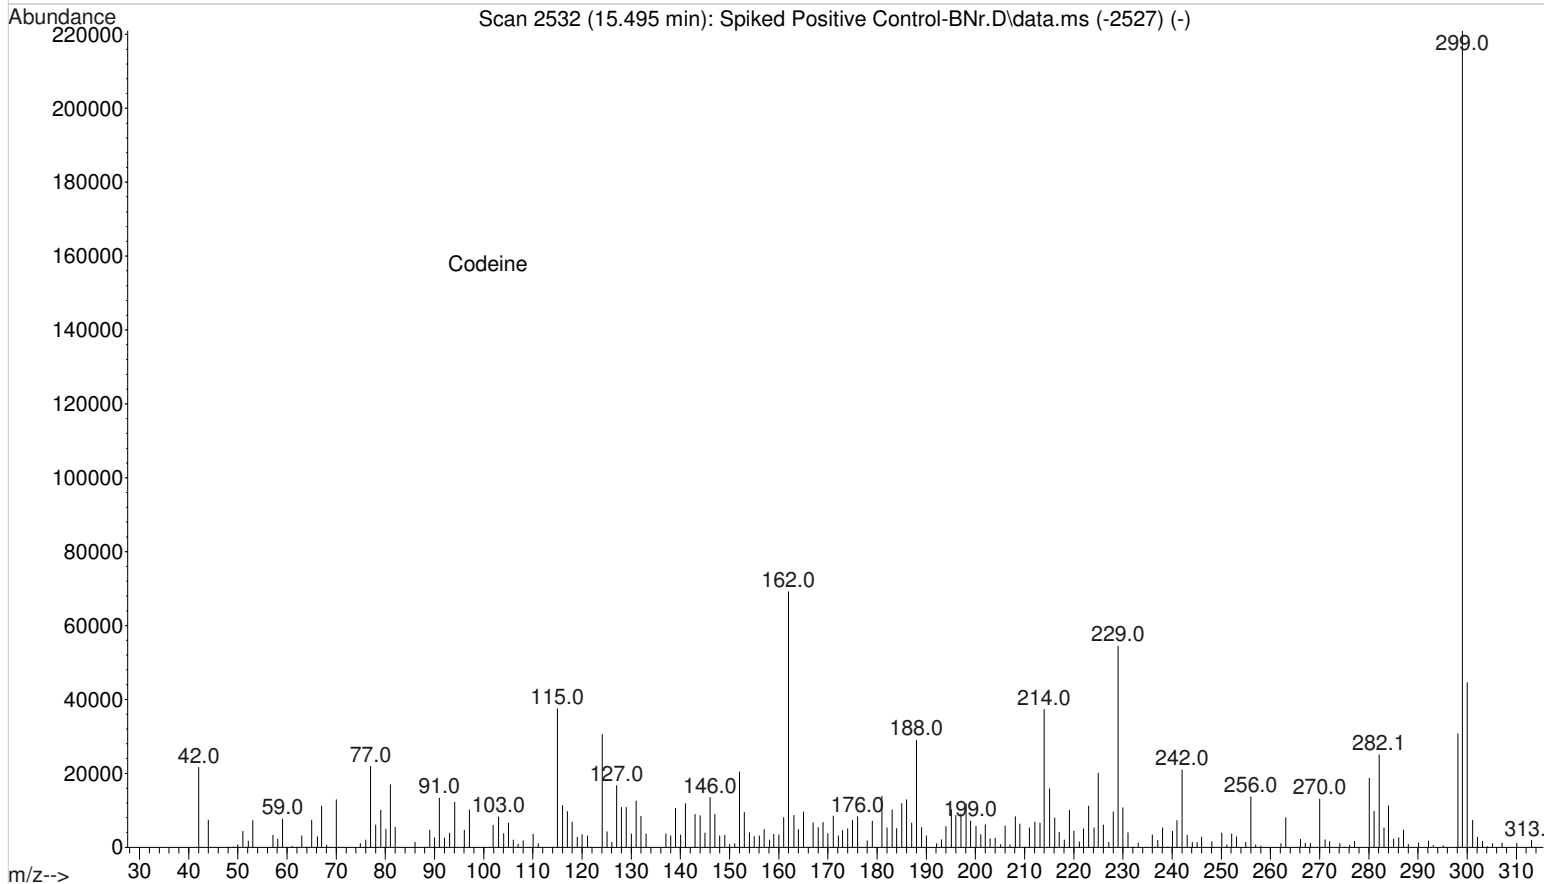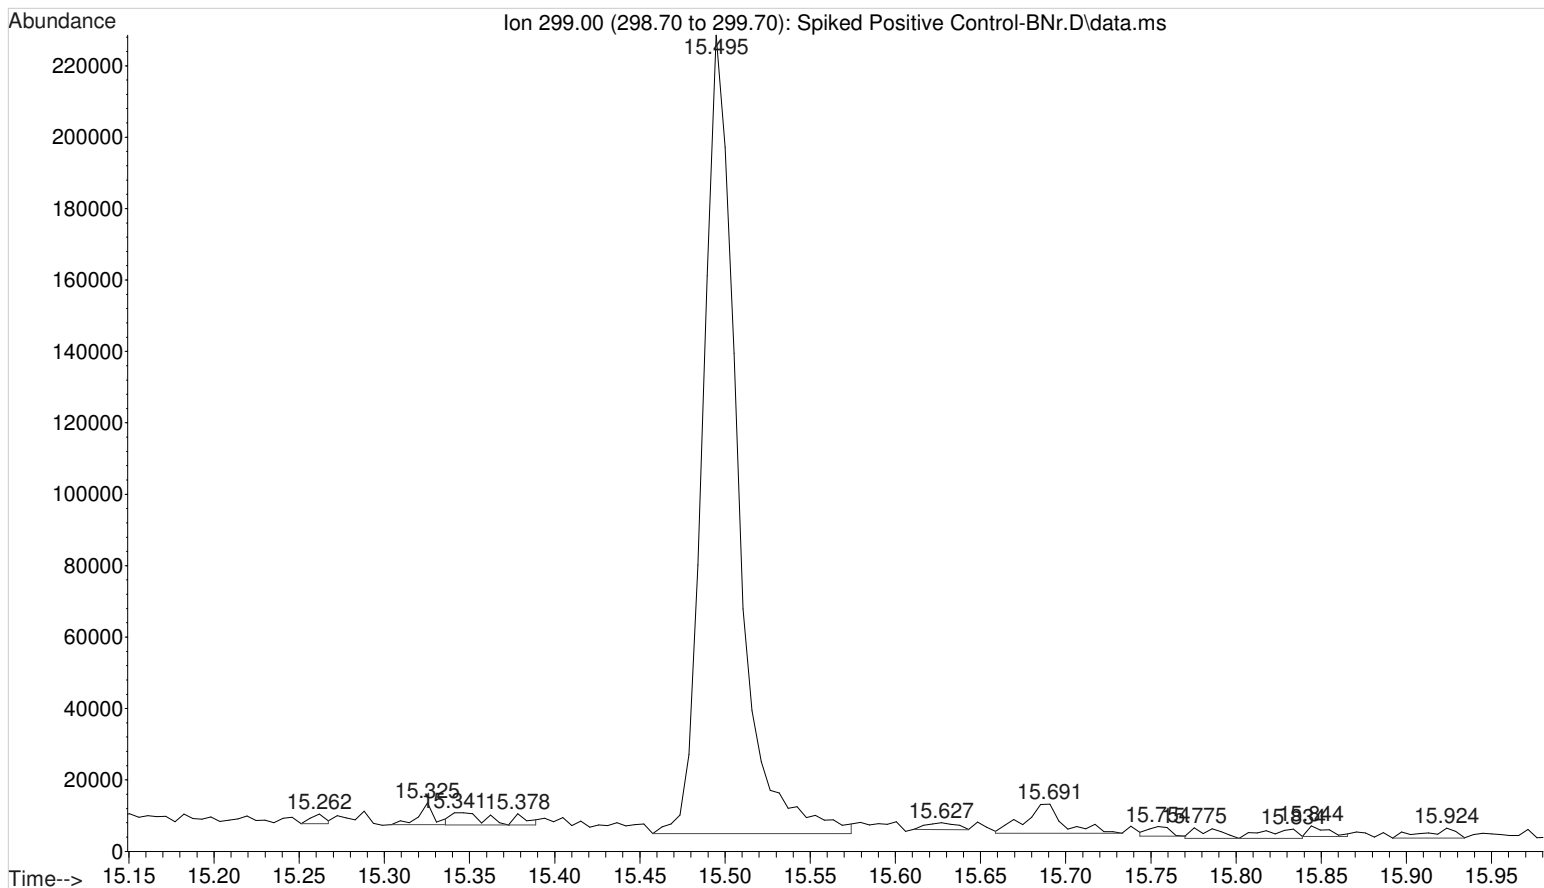

File : F:\10052016\10052016\10052016\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 05 Oct 2016 14:06 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name : Positive Control
Misc Info : UTAK B1013 + WS111215
Vial Number: 2

