


P2015-0904-1 was the only sample extracted - no worklist created. 

Simulate Run Sequence Mon May 11 11:12:24 2015

Instrument Name: Probie
 Sequence File: C:\msdchem\1\sequence\DD-BNSB051115.s
 Comment:
 Operator: D Downey
 Data Path: C:\MSDCHEM\1\DATA\DND\2015\051115BN\
 Method Path: C:\MSDCHEM\1\METHODS\

05/11/15

Line	Type	Vial	DataFile	Method	Sample Name
1)	Sample	100	Pre-run Solvent Blank		
	Datafile		Prerun Solvent Blank		
	Method		BNSB120510		
2)	Sample	1	Negative Control - Utak Lot B0689		
	Datafile		NegativeControl-BN		
	Method		BNSB120510		
3)	Sample	2	Positive Control		
	Datafile		SpikedPositiveControl-BN		
	Method		BNSB120510		
4)	Sample	99	Solvent Blank		
	Datafile		prbLK2		
	Method		BNSB120510		
5)	Sample	100	Pre-run Solvent Blank		
	Datafile		Prerun Solvent Blankr		
	Method		GBT092509		
6)	Sample	1	Negative Control - Utak Lot B0689		
	Datafile		NegativeControl-BNr		
	Method		GBT092509		
7)	Sample	2	Positive Control		
	Datafile		SpikedPositiveControl-BNr		
	Method		GBT092509		
8)	Sample	99	Solvent Blank		
	Datafile		prbLK2r		
	Method		GBT092509		
9)	Sample	98	Lab No.: P2015-0904-1		
	Datafile		P2015-0904-1-BNBLK		
	Method		BNSB120510		
10)	Sample	3	Lab No.: P2015-0904-1		
	Datafile		P2015-0904-1-BN		
	Method		BNSB120510		
11)	Sample	98	Lab No.: P2015-0904-1		
	Datafile		P2015-0904-1-BNBLKr		
	Method		GBT092509		
12)	Sample	3	Lab No.: P2015-0904-1		
	Datafile		P2015-0904-1-BNr		
	Method		GBT092509		
13)	Sample	97	BLK		
	Datafile		POSTBLKr		
	Method		GBT092509		
14)	Sample	96	BLK		
	Datafile		AFTER		
	Method		BNSB120510		


Bytes Needed: 63815423 Space on drive C: 4.36072e+011
 Sequence Verification Done!

Analytical Method 3.6.1 & 3.6.7 QA Check List

Run Start Date: 05/11/15

Analyst: DND

(Short GC/MS temperature program)



Positive Control Compound List


- Methamphetamine
- Nicotine
- Meperidine
- Caffeine
- Diphenhydramine
- Lidocaine
- PCP
- Methadone
- Amitriptyline
- Codeine
- Trazodone

Internal Standards


- Benzphetamine
- Papaverine

Optional back extraction **not** performed.
Samples reconstituted in methanol.



File :C:\gcms\1\data\Blood\051115BN\Prerun Solvent Blank.D
Operator : D Downey
Acquired : 11 May 2015 16:49 using AcqMethod BNSB120510.M
Instrument : Probie
Sample Name: Pre-run Solvent Blank
Misc Info : Chloroform
Vial Number: 100

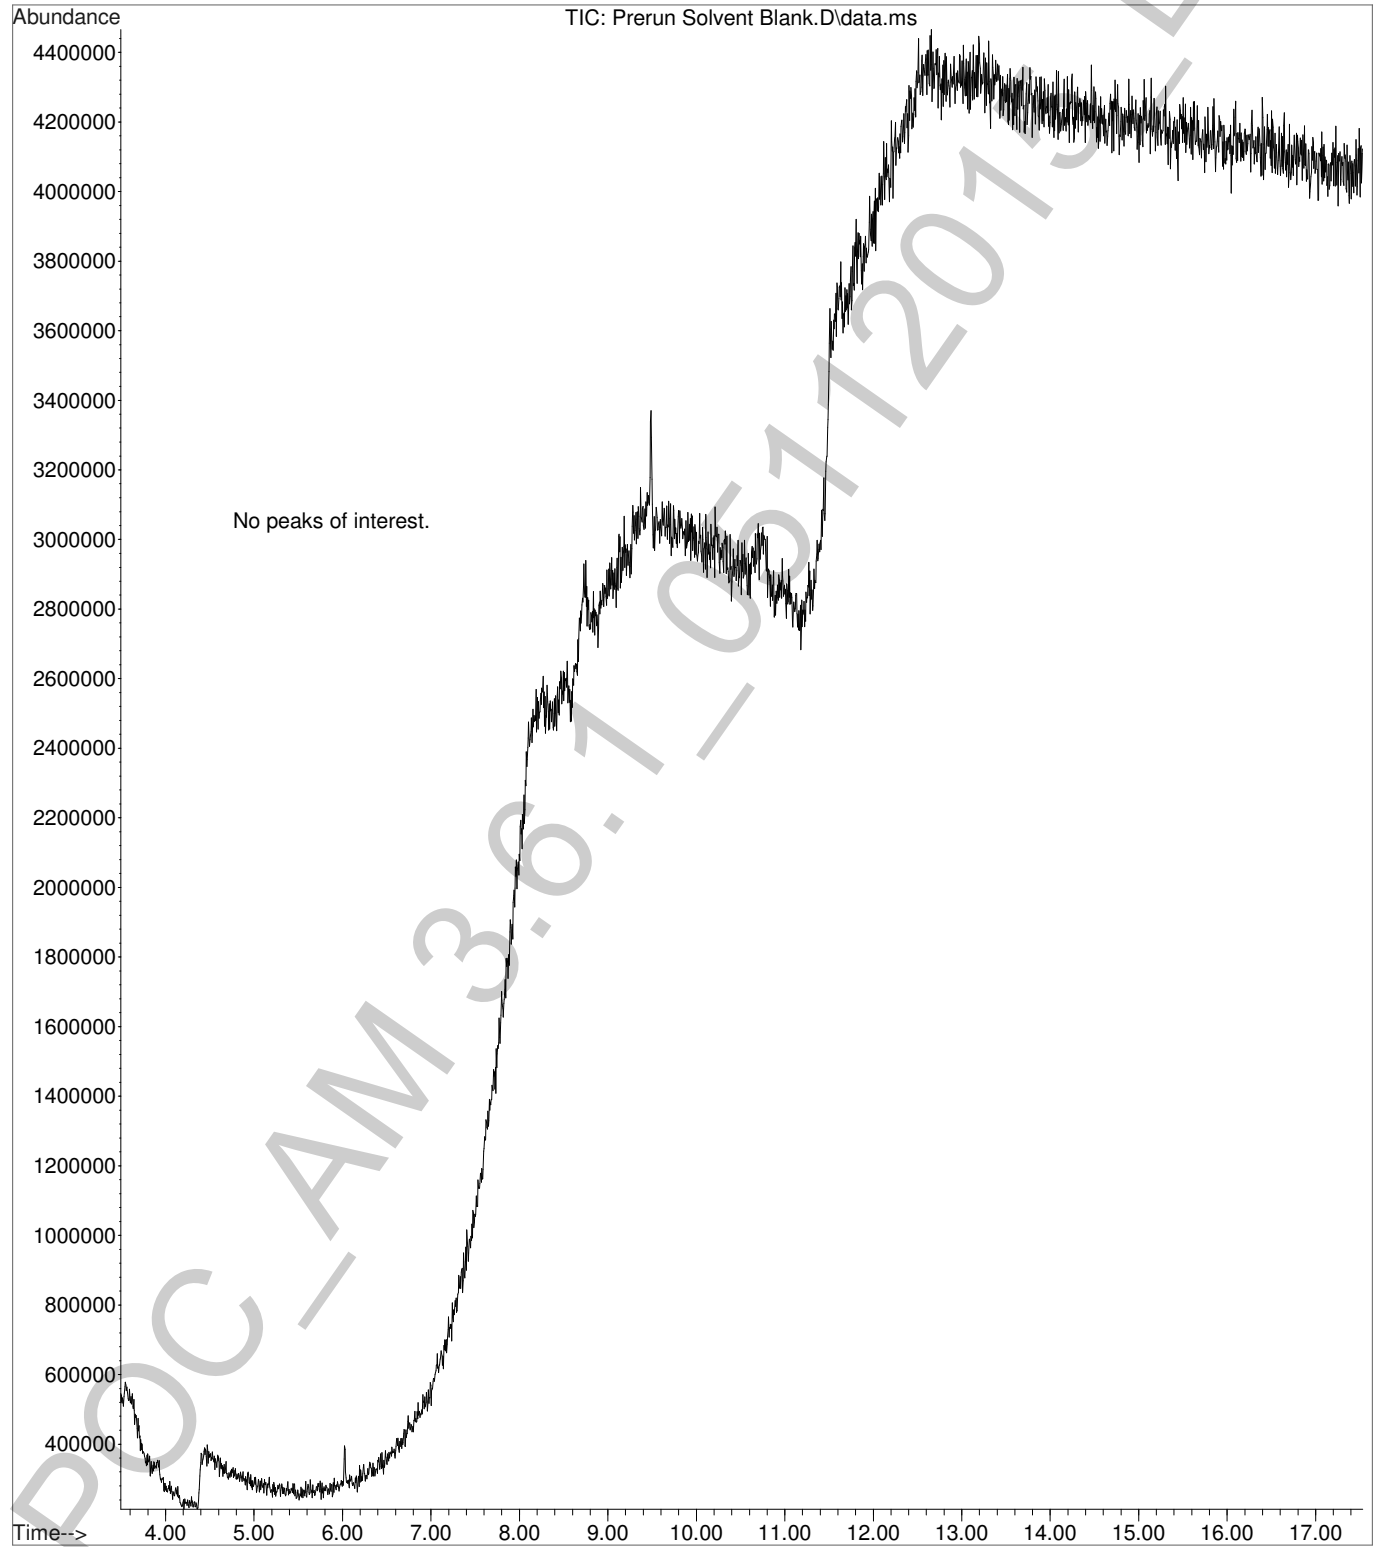



File :C:\gcms\1\data\Blood\051115BN\NegativeControl-BN.D
Operator : D Downey
Acquired : 11 May 2015 17:12 using AcqMethod BNSB120510.M
Instrument : Probie
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1
Vial Number: 1

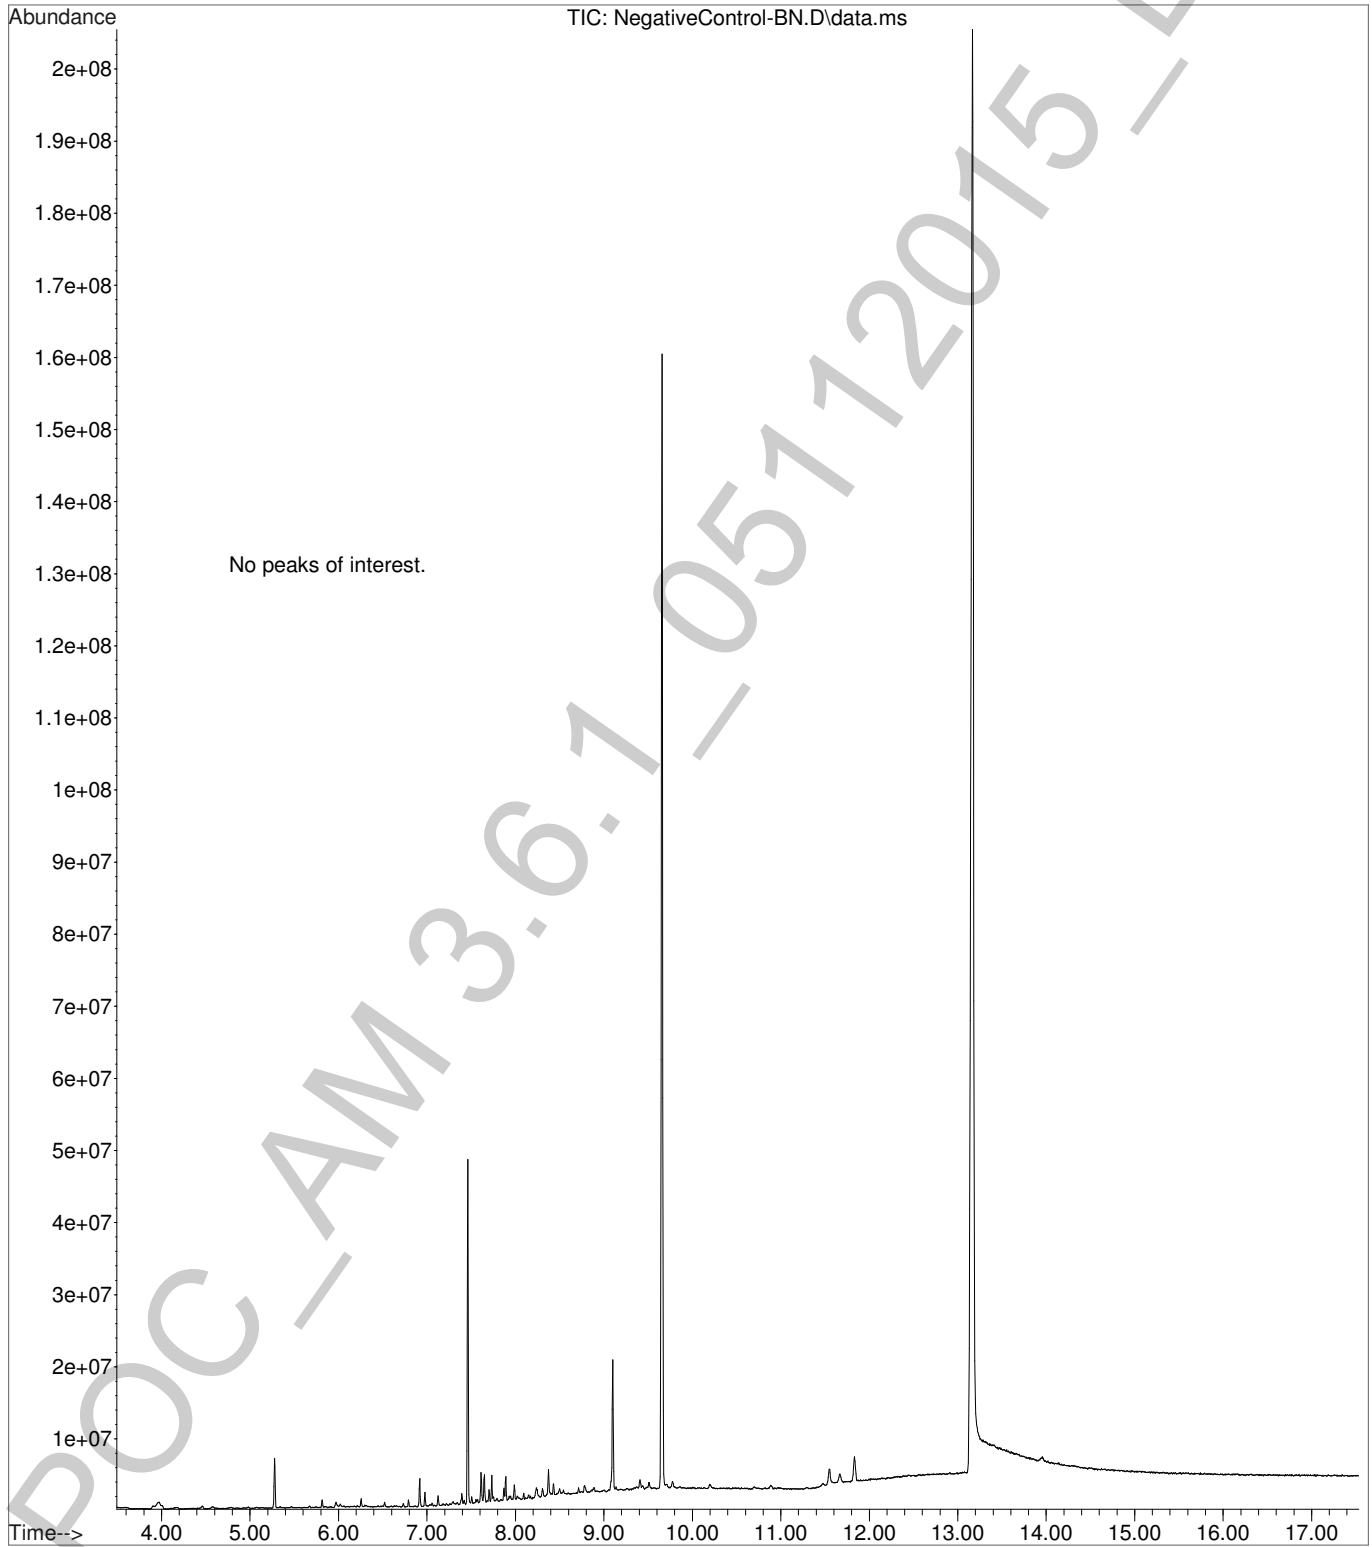


File :C:\gcms\1\data\Blood\051115BN\NegativeControl-BN.D
Operator : D Downey
Acquired : 11 May 2015 17:12 using AcqMethod BNSB120510.M
Instrument : Probie
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1
Vial Number: 1

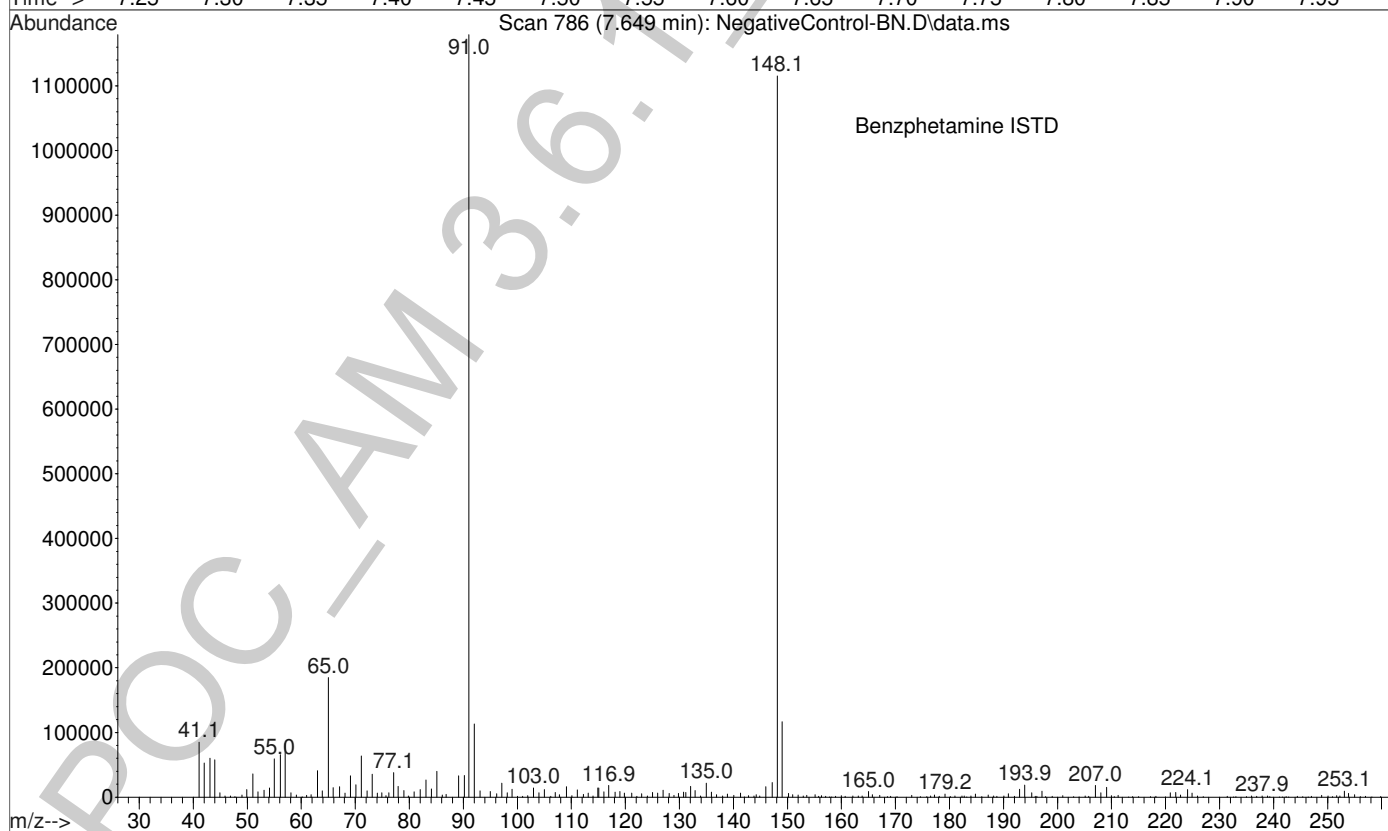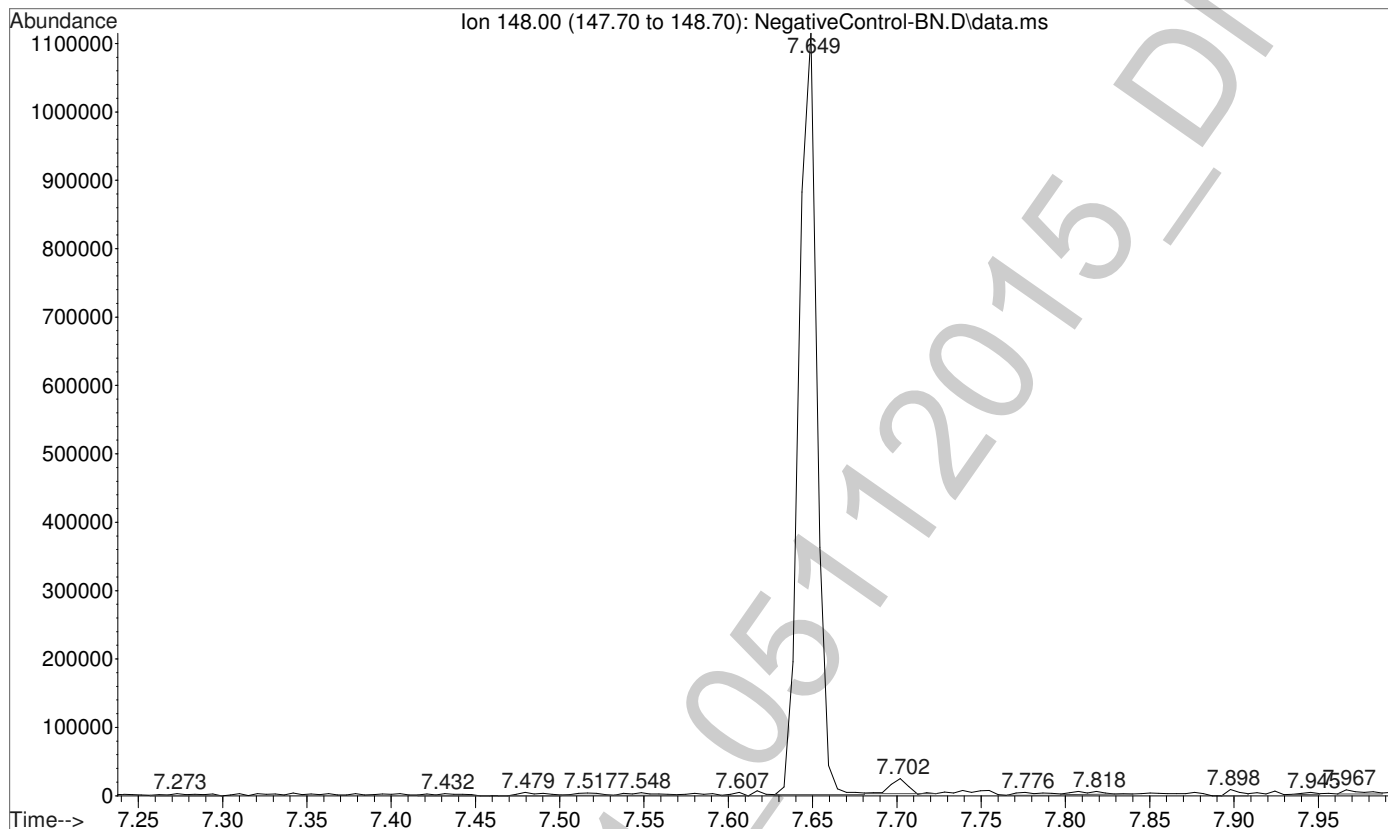



File :C:\gcms\1\data\Blood\051115BN\NegativeControl-BN.D
Operator : D Downey
Acquired : 11 May 2015 17:12 using AcqMethod BNSB120510.M
Instrument : Probie
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1
Vial Number: 1

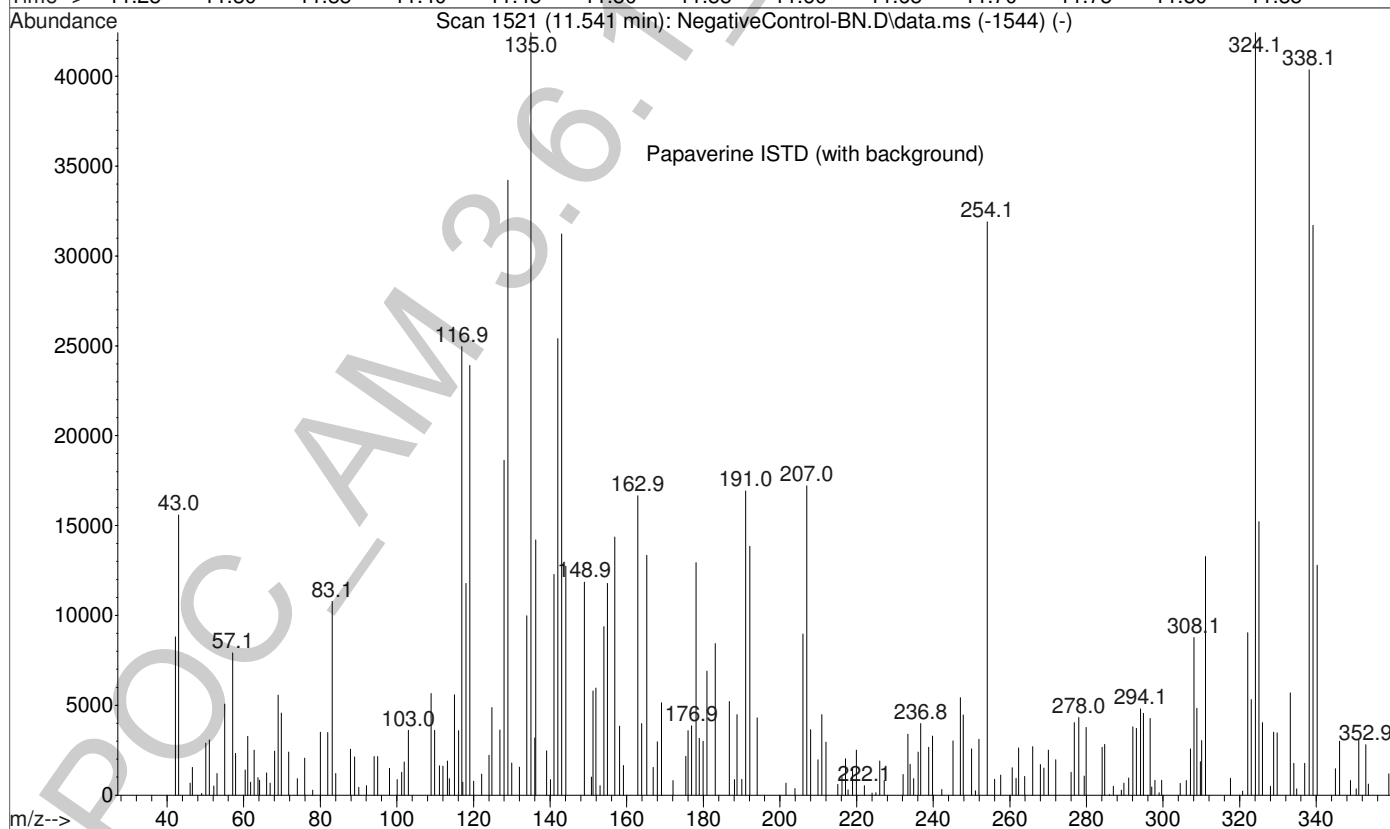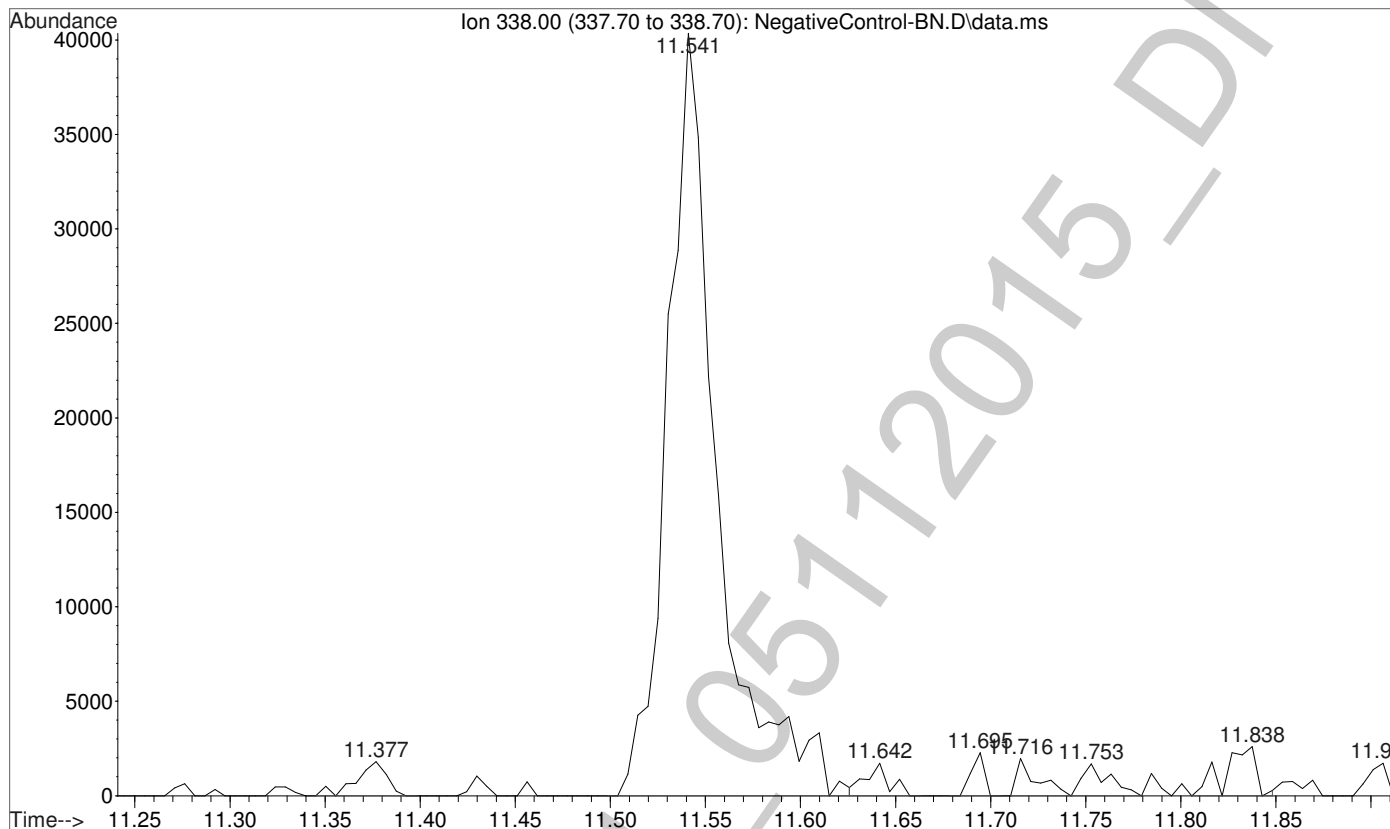



File :C:\gcms\1\data\Blood\051115BN\SpikedPositiveControl-BN.D
Operator : D Downey
Acquired : 11 May 2015 17:36 using AcqMethod BNSB120510.M
Instrument : Probie
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

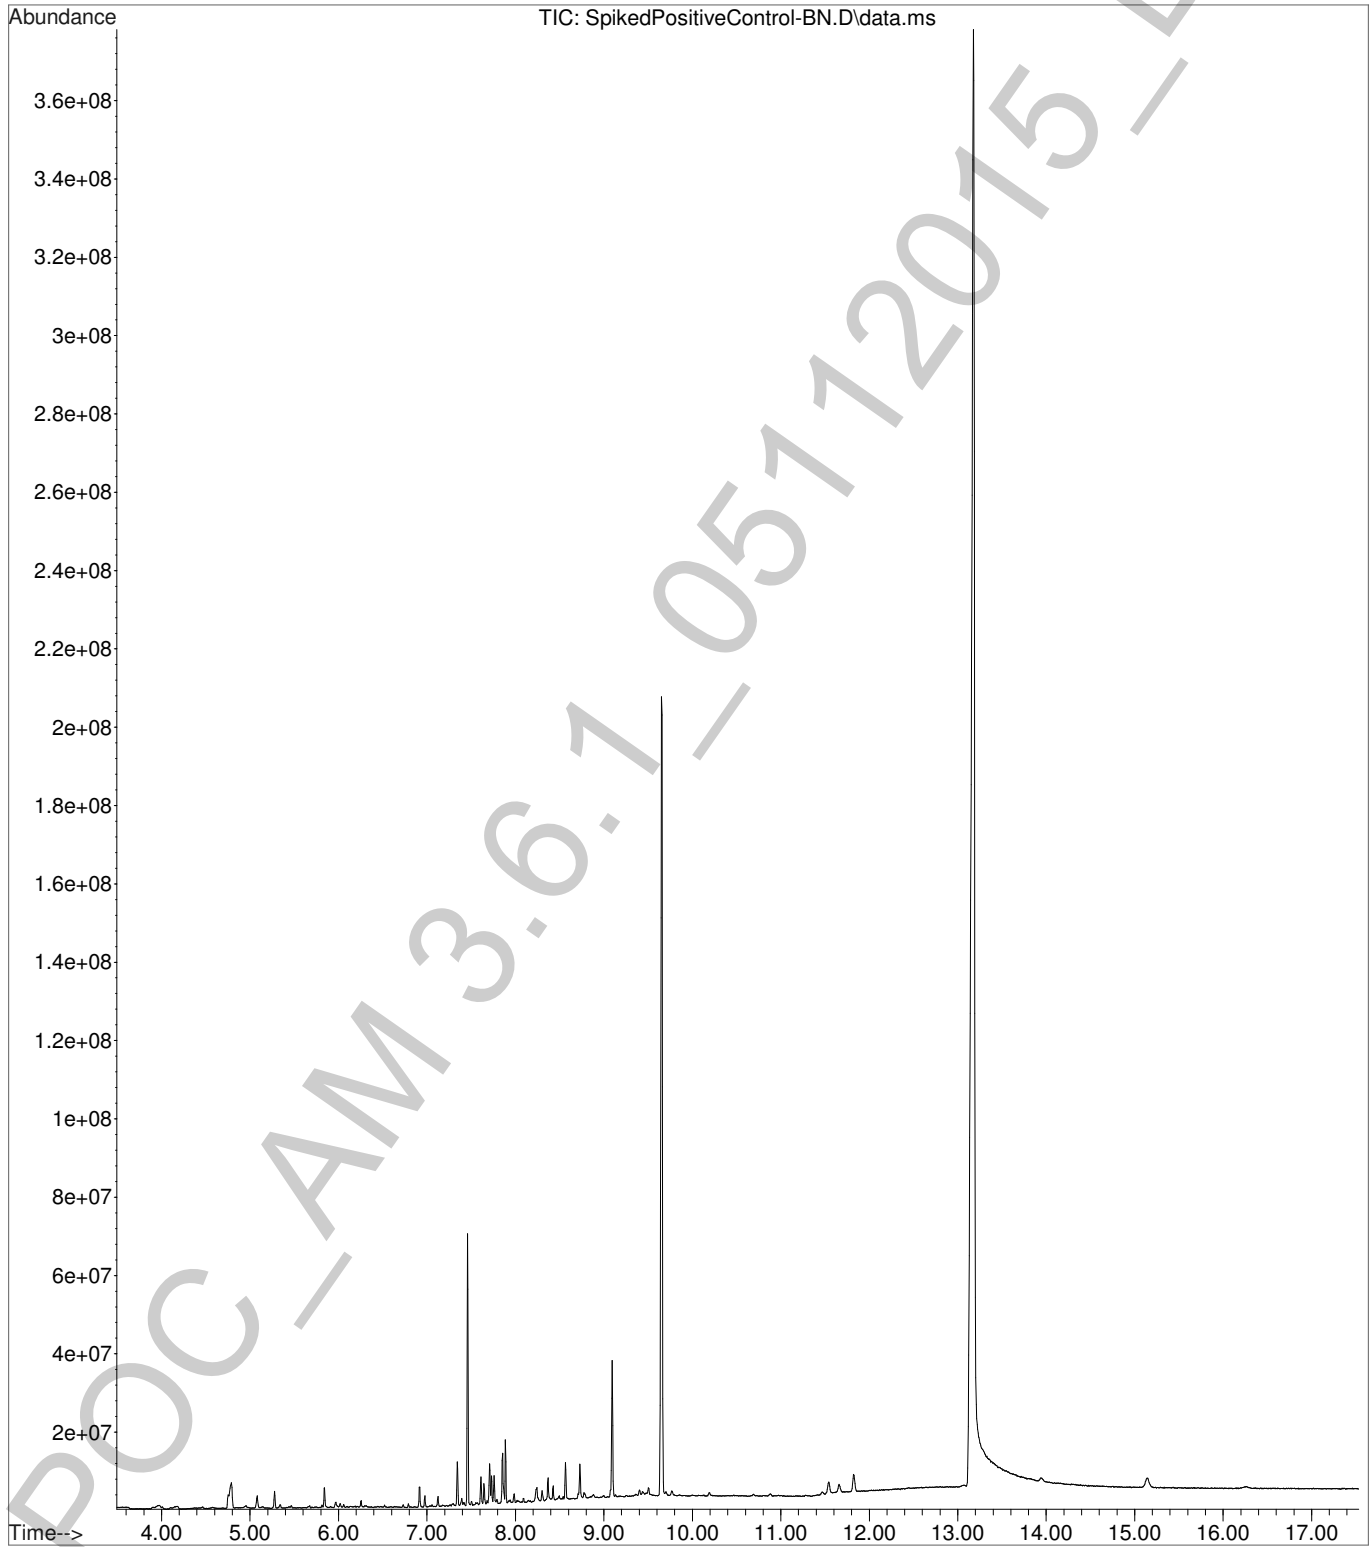



File :C:\gcms\1\data\Blood\051115BN\SpikedPositiveControl-BN.D
Operator : D Downey
Acquired : 11 May 2015 17:36 using AcqMethod BNSB120510.M
Instrument : Probie
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

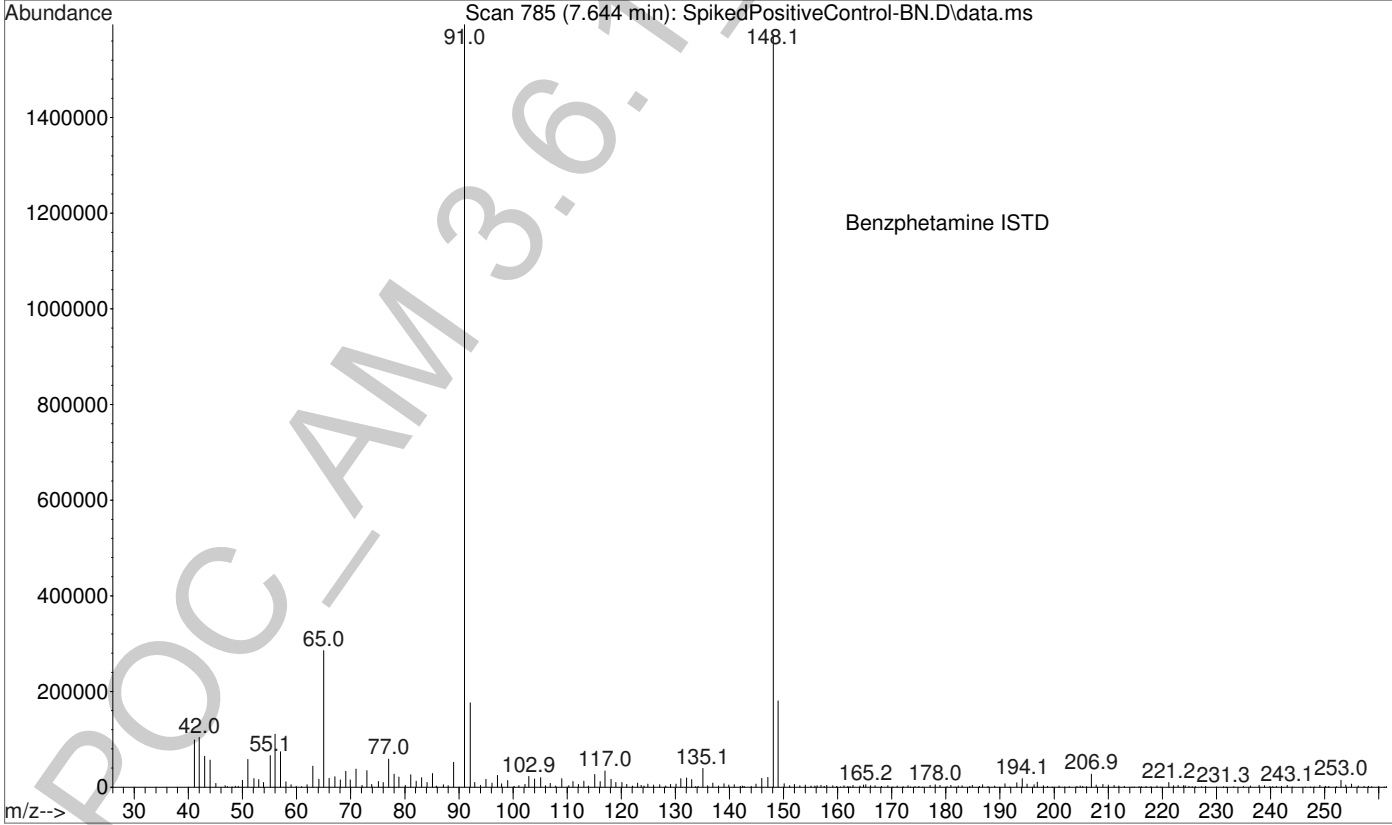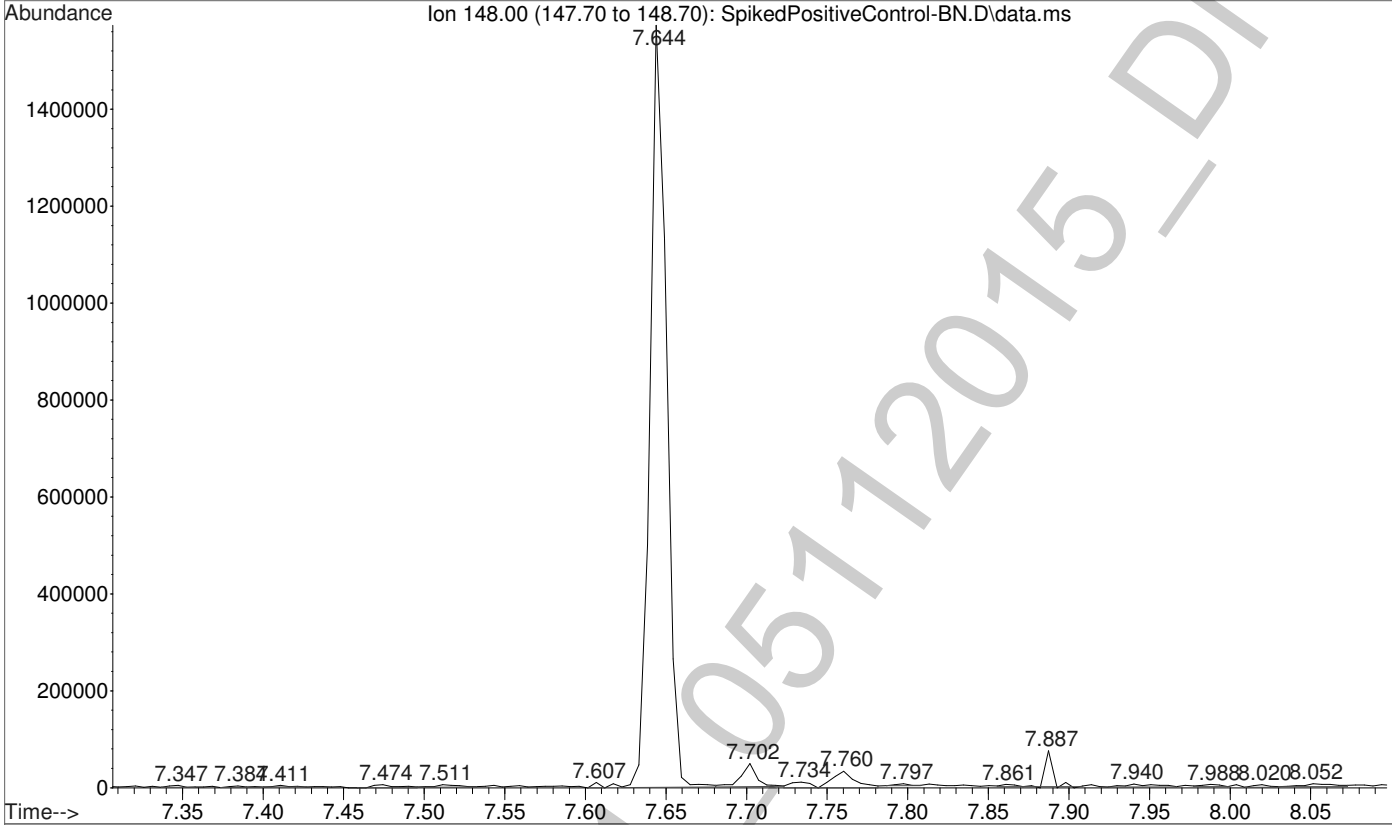



File :C:\gcms\1\data\Blood\051115BN\SpikedPositiveControl-BN.D
Operator : D Downey
Acquired : 11 May 2015 17:36 using AcqMethod BNSB120510.M
Instrument : Probie
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

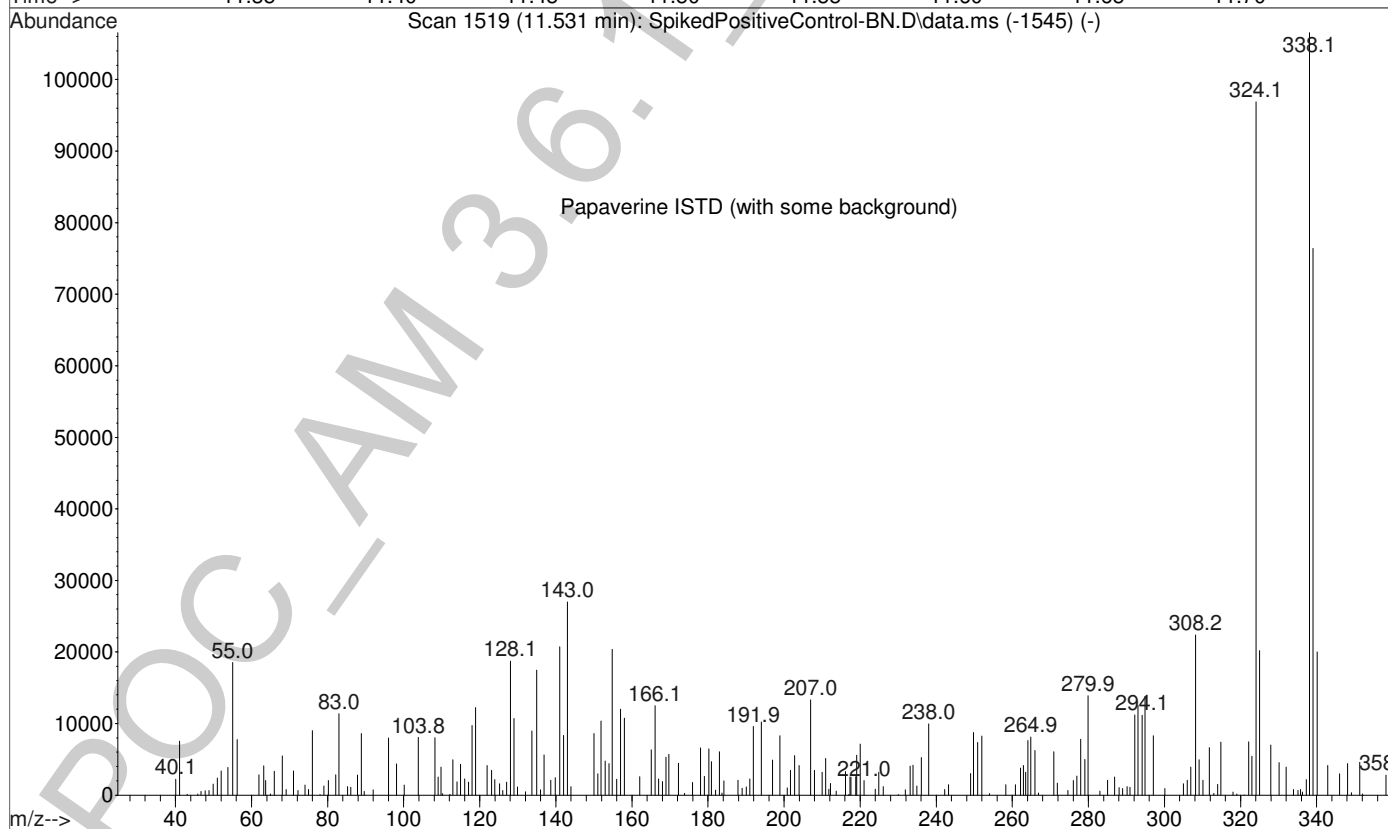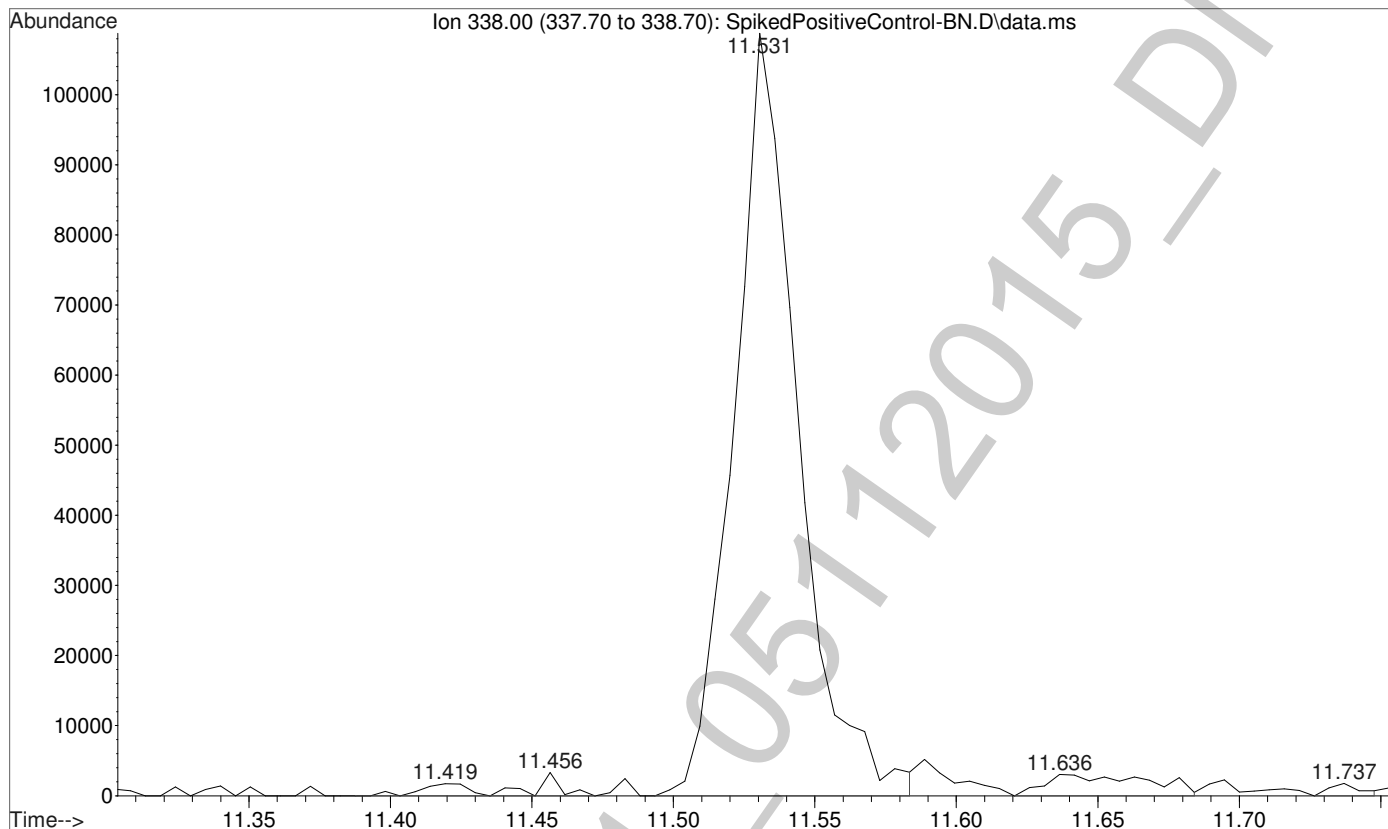



File :C:\gcms\1\data\Blood\051115BN\SpikedPositiveControl-BN.D
Operator : D Downey
Acquired : 11 May 2015 17:36 using AcqMethod BNSB120510.M
Instrument : Probie
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

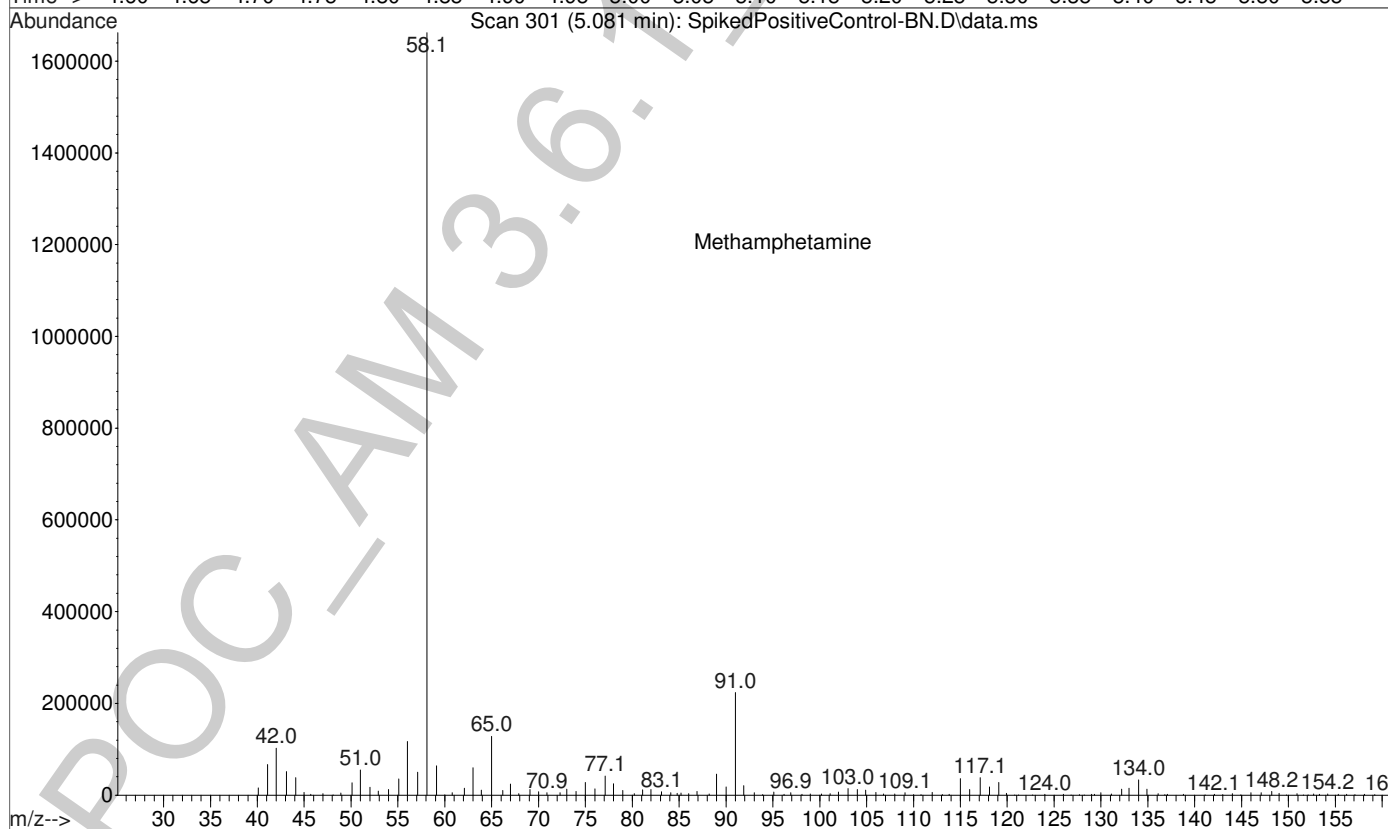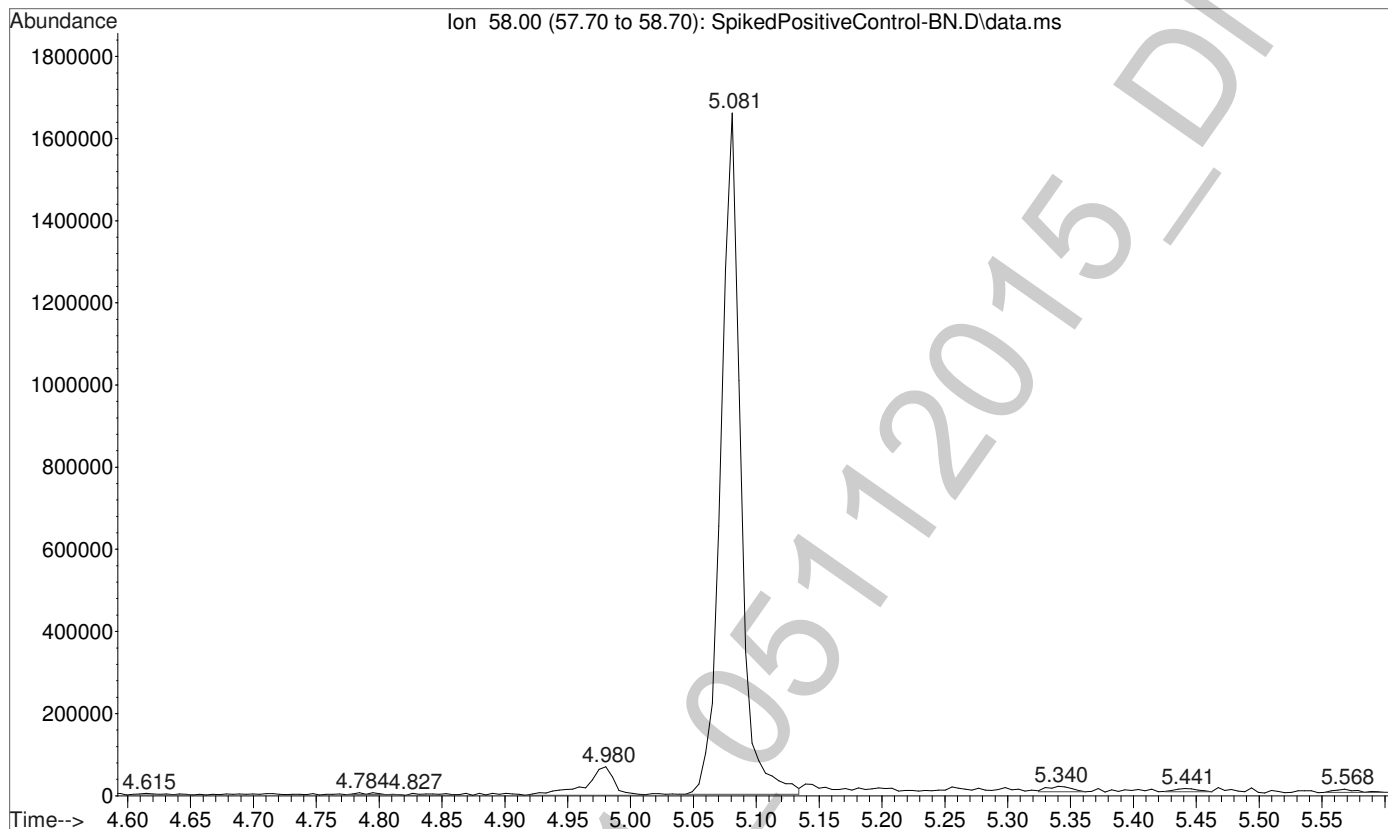



File :C:\gcms\1\data\Blood\051115BN\SpikedPositiveControl-BN.D
Operator : D Downey
Acquired : 11 May 2015 17:36 using AcqMethod BNSB120510.M
Instrument : Probie
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

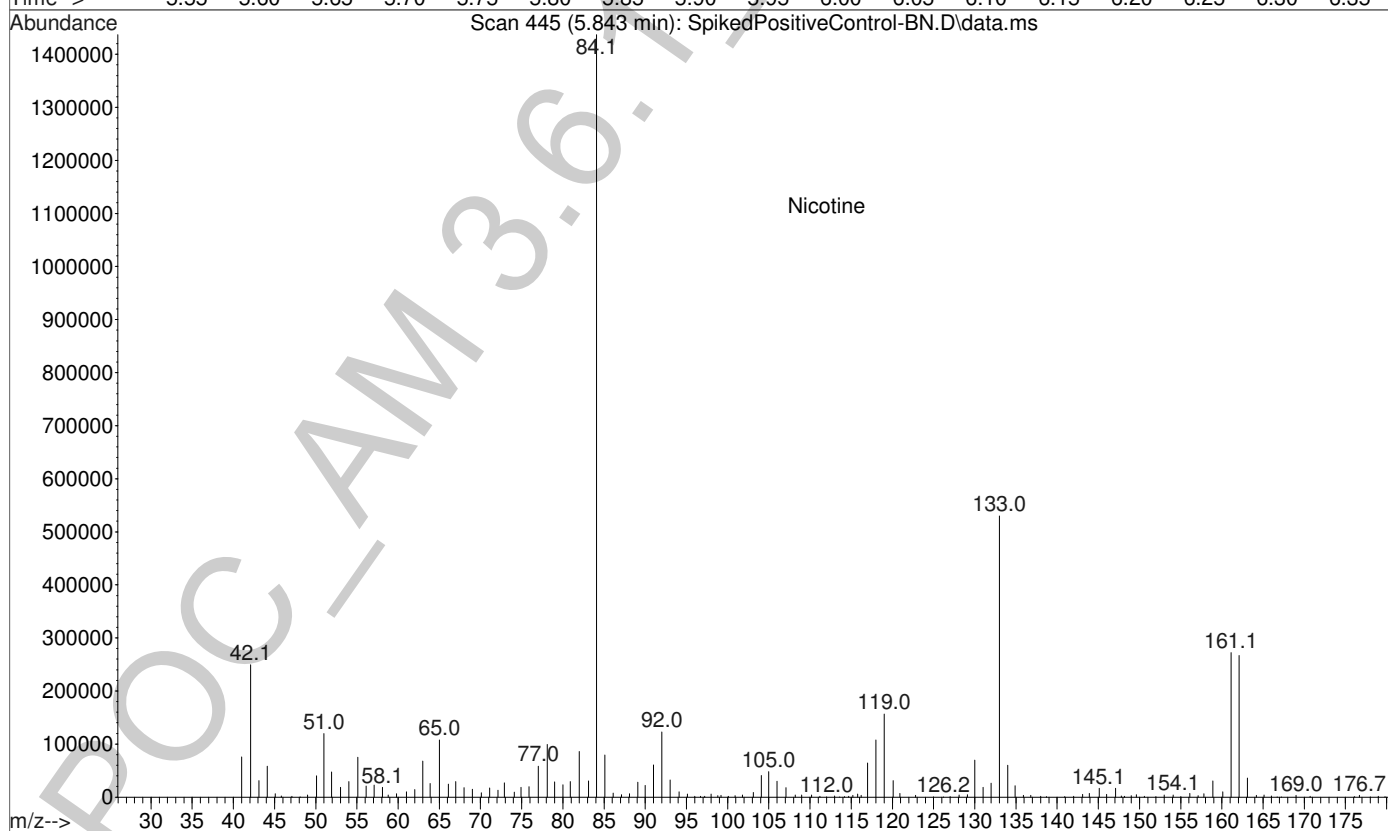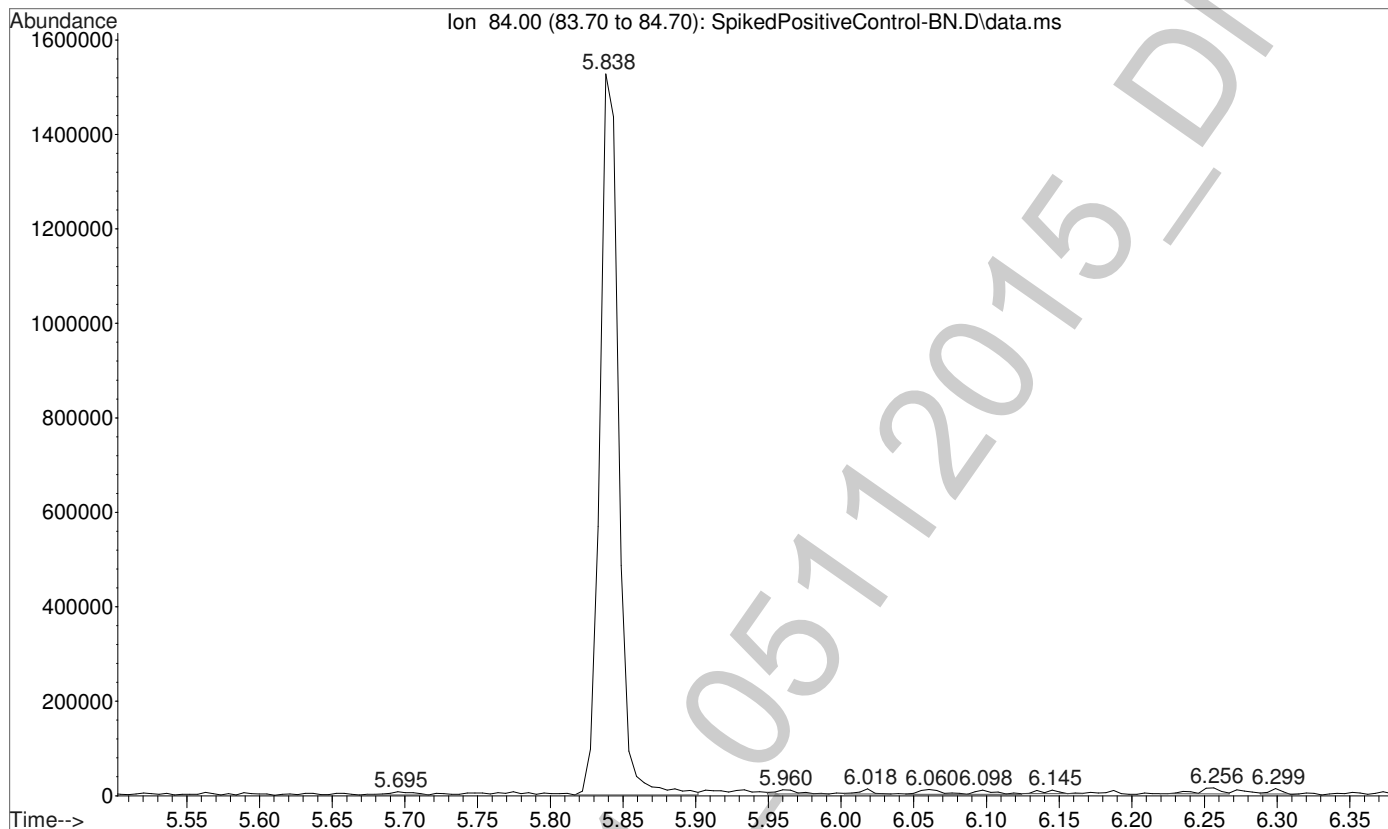



File :C:\gcms\1\data\Blood\051115BN\SpikedPositiveControl-BN.D
Operator : D Downey
Acquired : 11 May 2015 17:36 using AcqMethod BNSB120510.M
Instrument : Probie
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

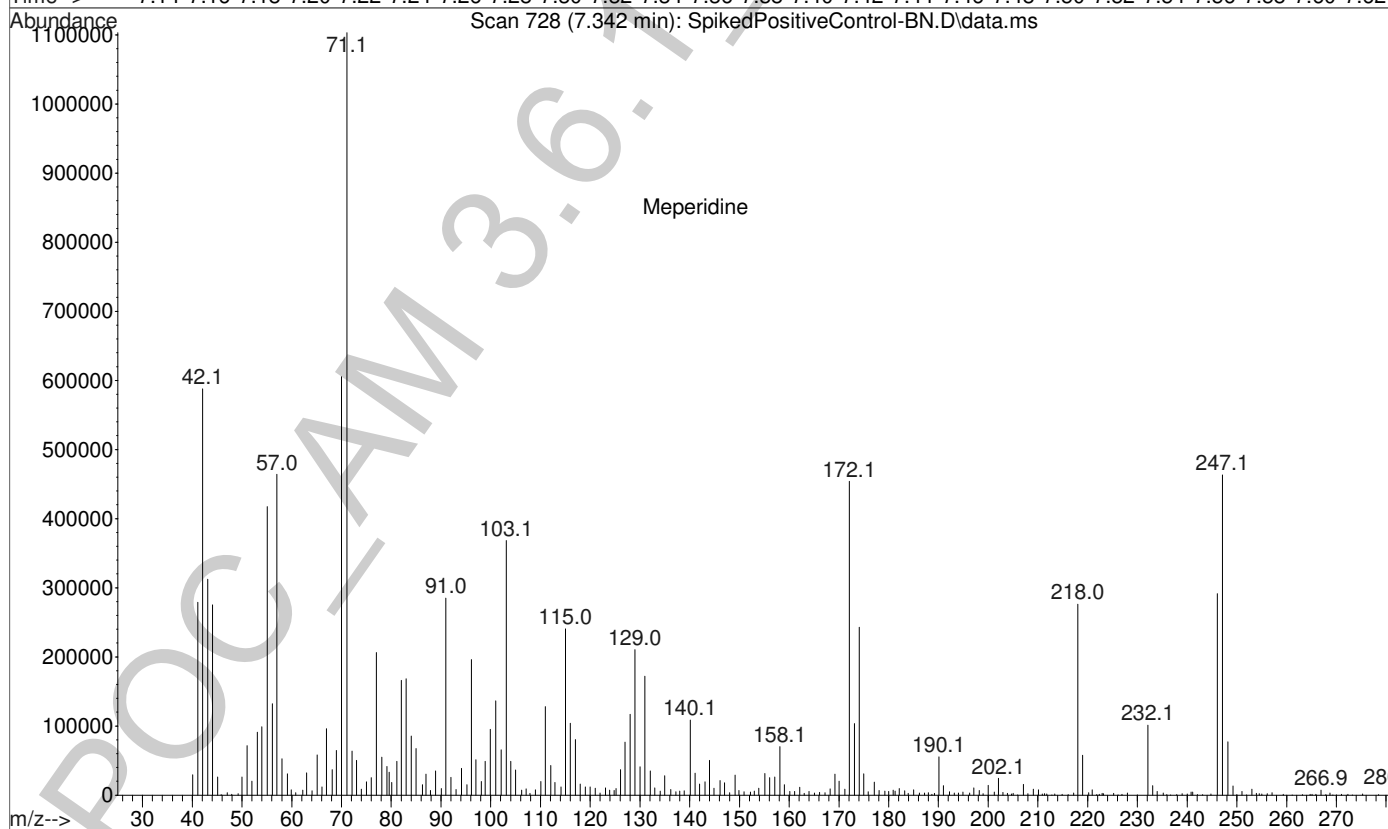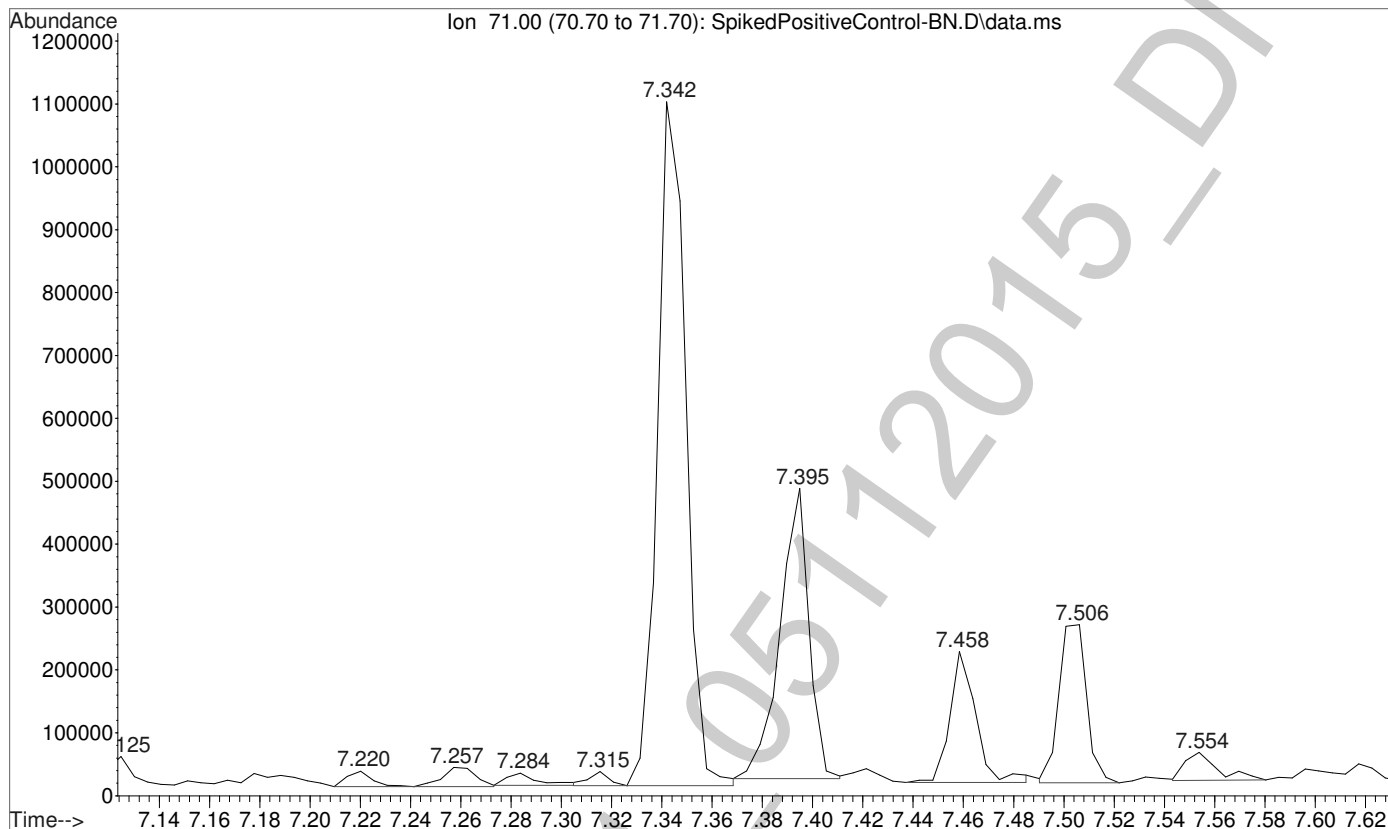


File :C:\gcms\1\data\Blood\051115BN\SpikedPositiveControl-BN.D
Operator : D Downey
Acquired : 11 May 2015 17:36 using AcqMethod BNSB120510.M
Instrument : Probie
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

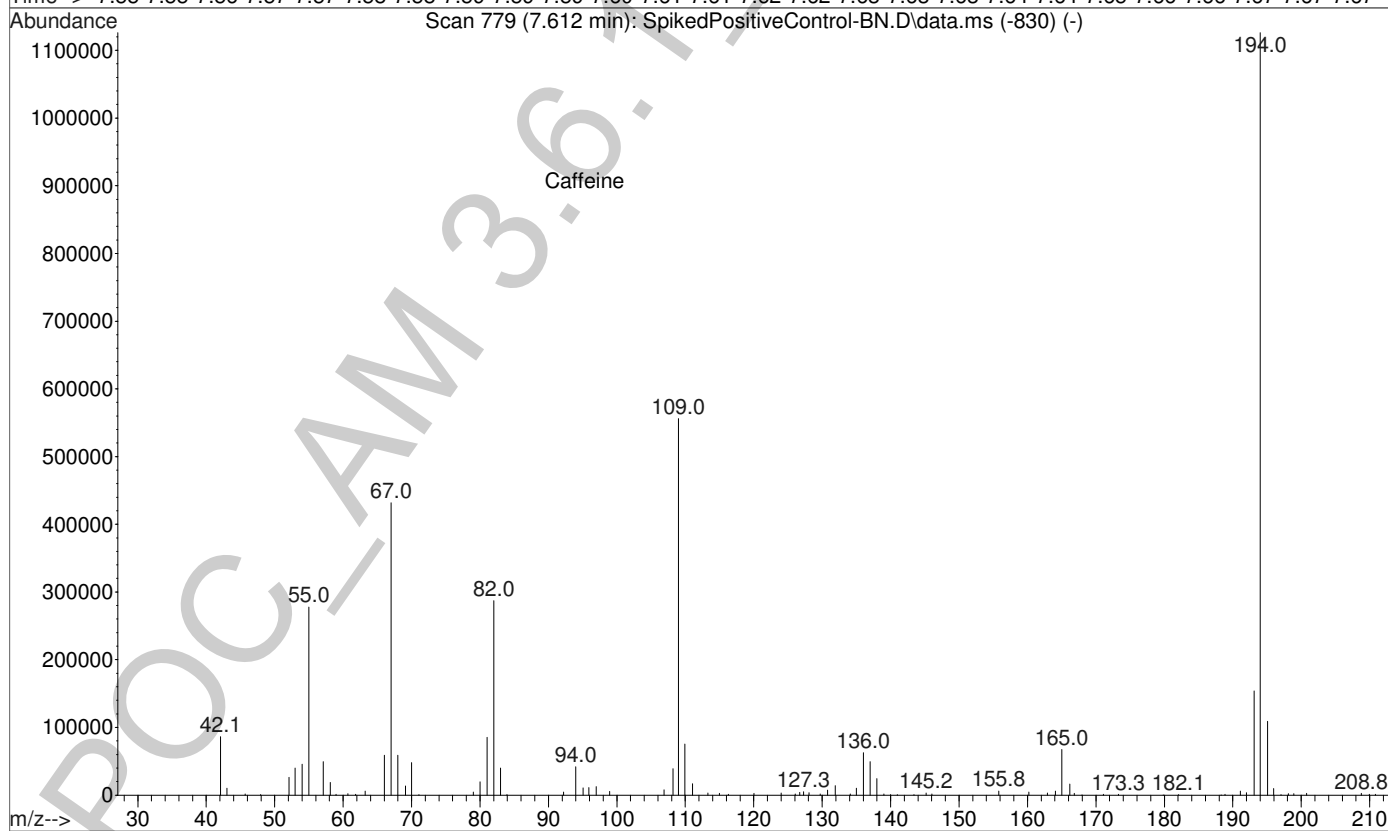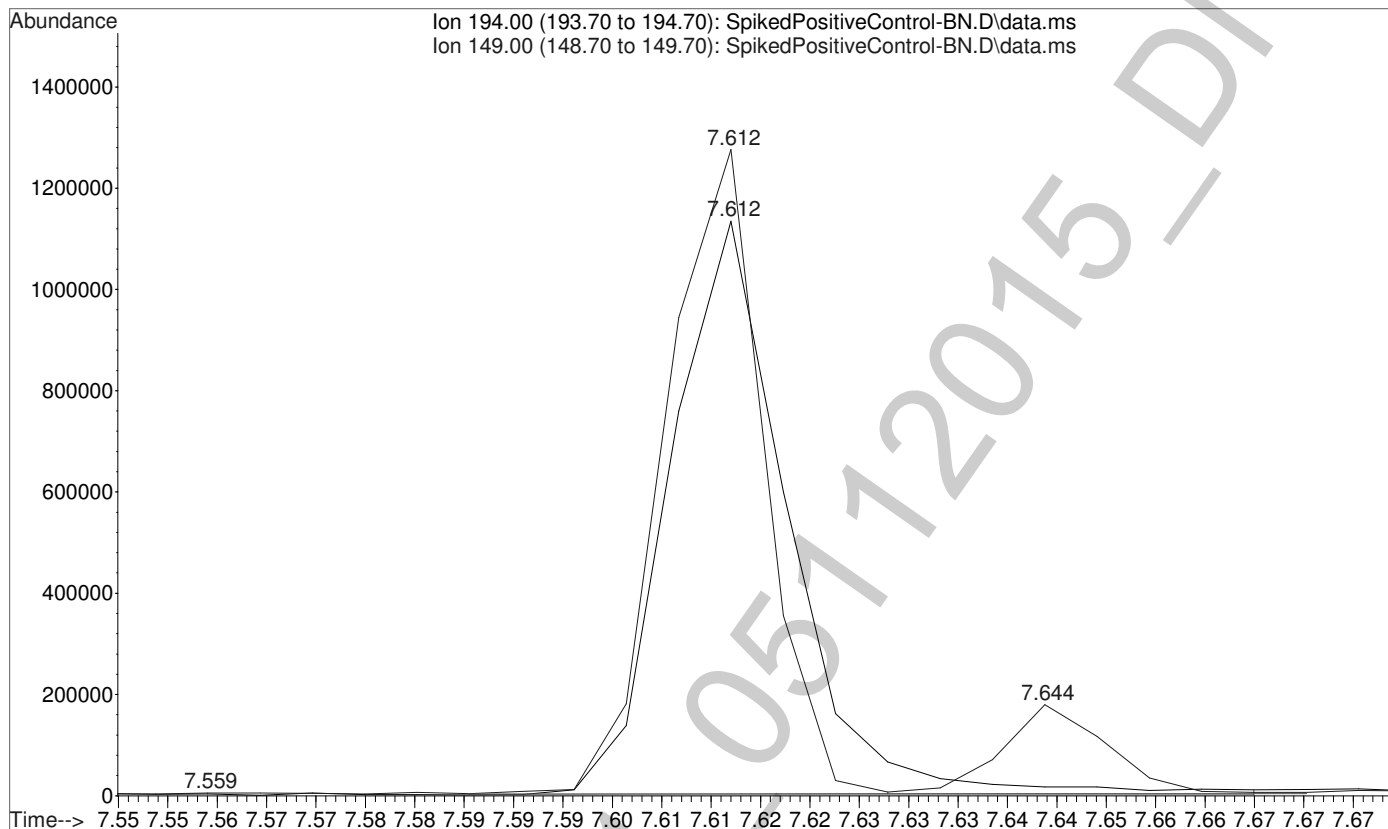



File :C:\gcms\1\data\Blood\051115BN\SpikedPositiveControl-BN.D
Operator : D Downey
Acquired : 11 May 2015 17:36 using AcqMethod BNSB120510.M
Instrument : Probie
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

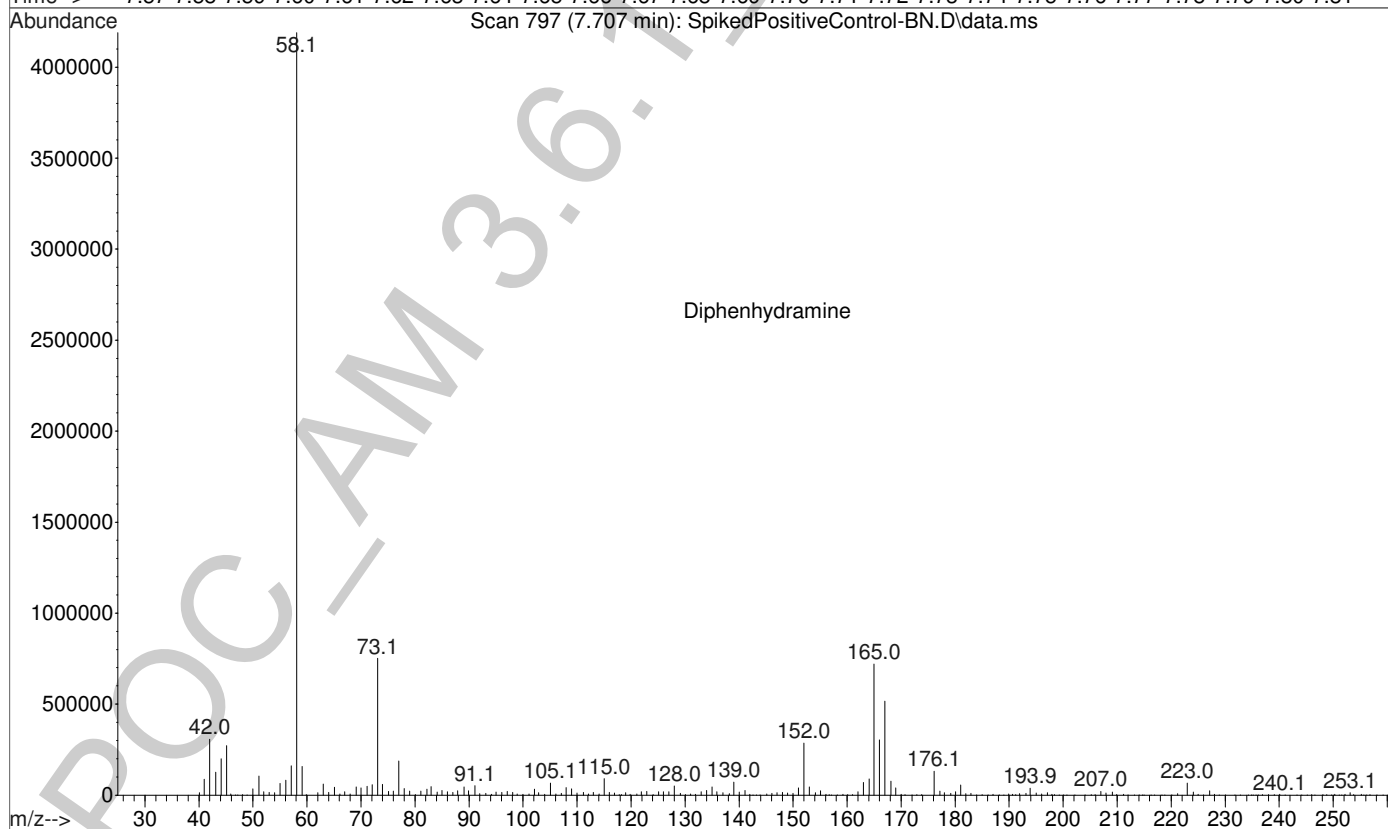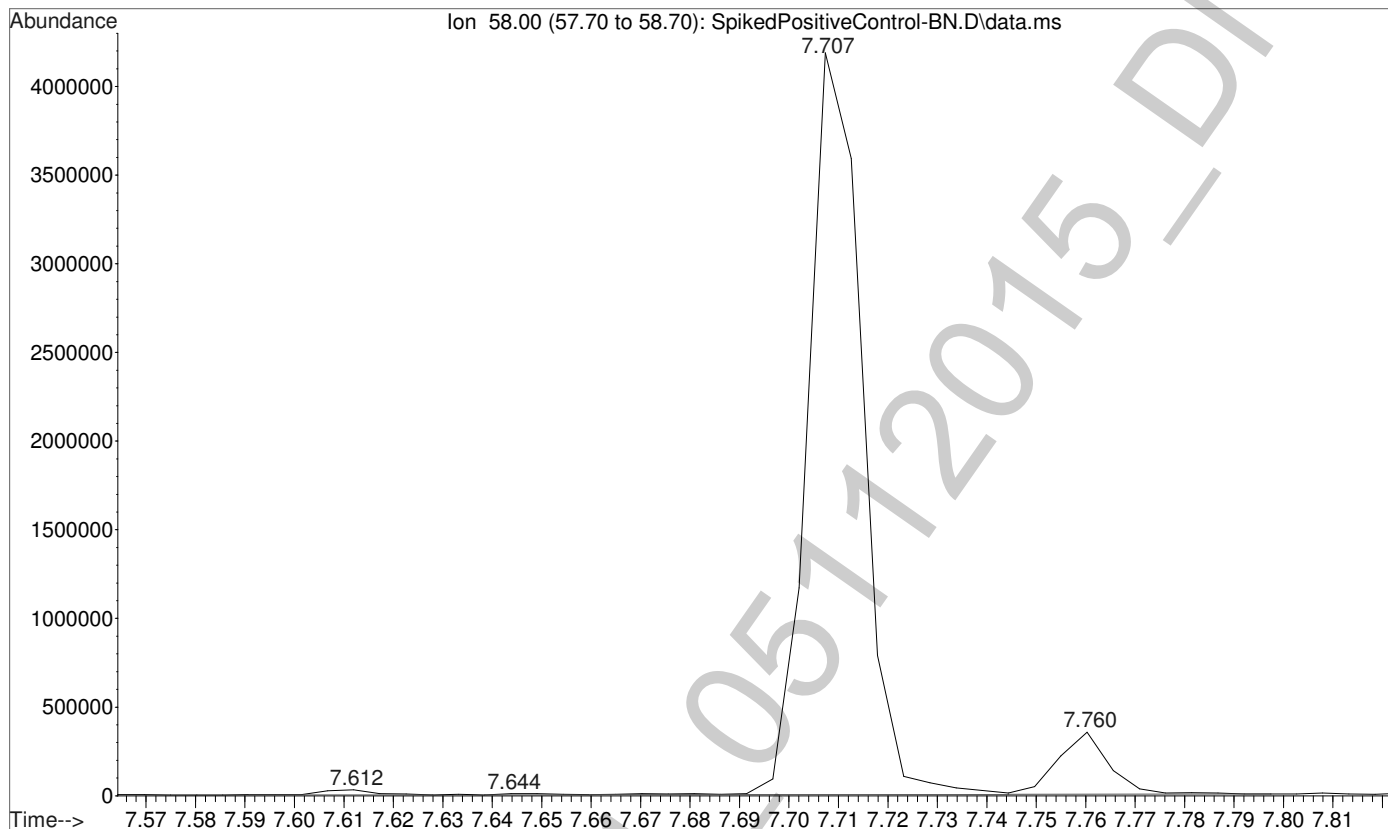



File :C:\gcms\1\data\Blood\051115BN\SpikedPositiveControl-BN.D
Operator : D Downey
Acquired : 11 May 2015 17:36 using AcqMethod BNSB120510.M
Instrument : Probie
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

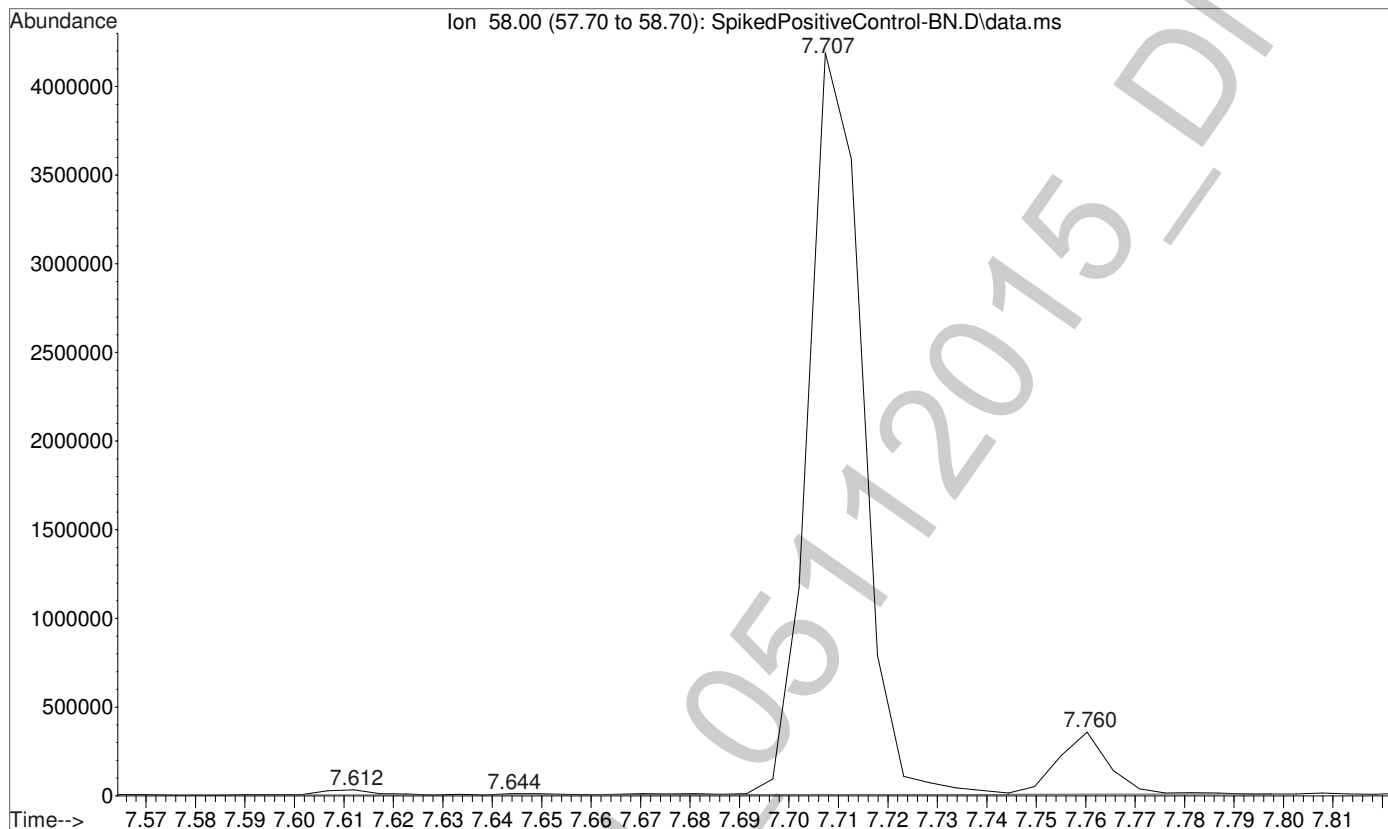



File :C:\gcms\1\data\Blood\051115BN\SpikedPositiveControl-BN.D
Operator : D Downey
Acquired : 11 May 2015 17:36 using AcqMethod BNSB120510.M
Instrument : Probie
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

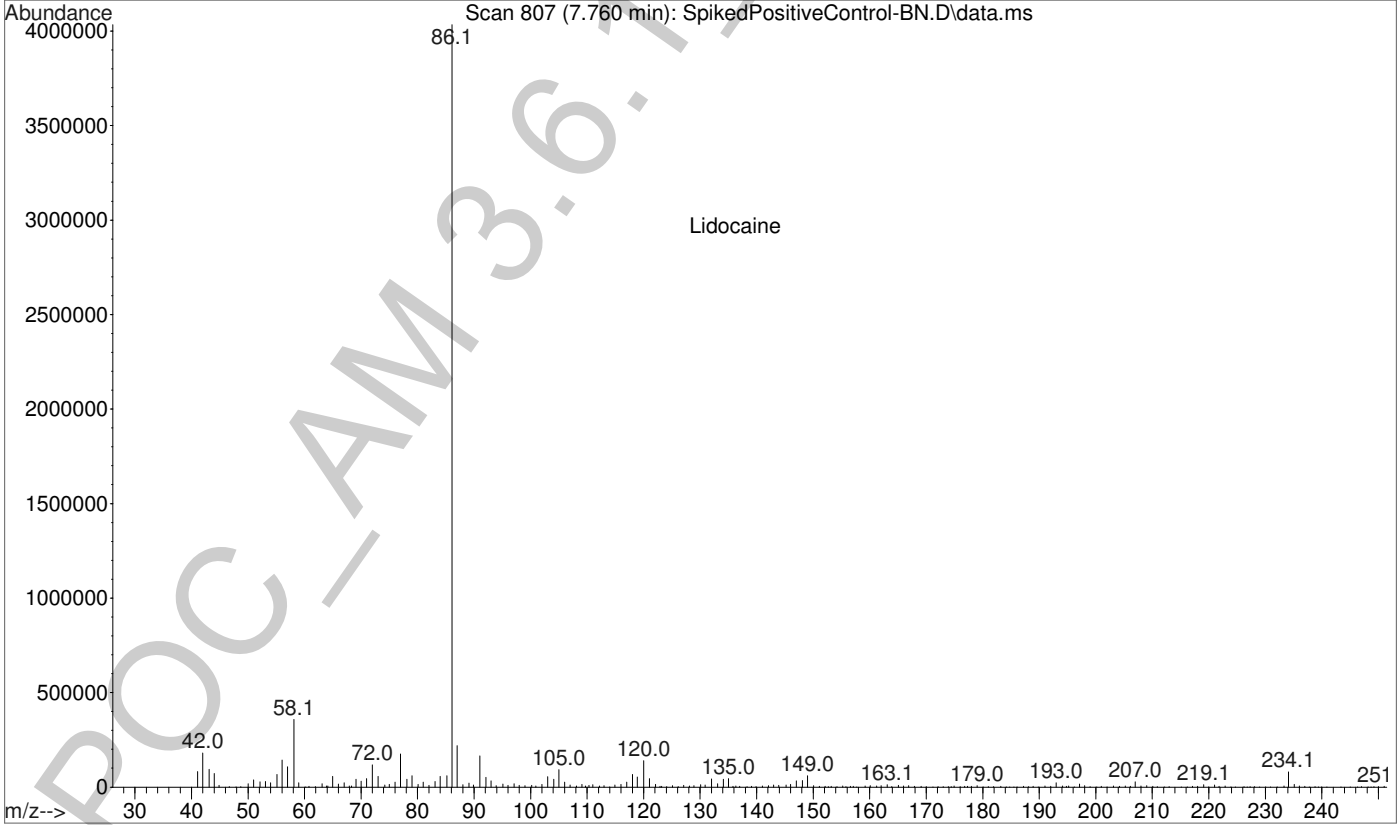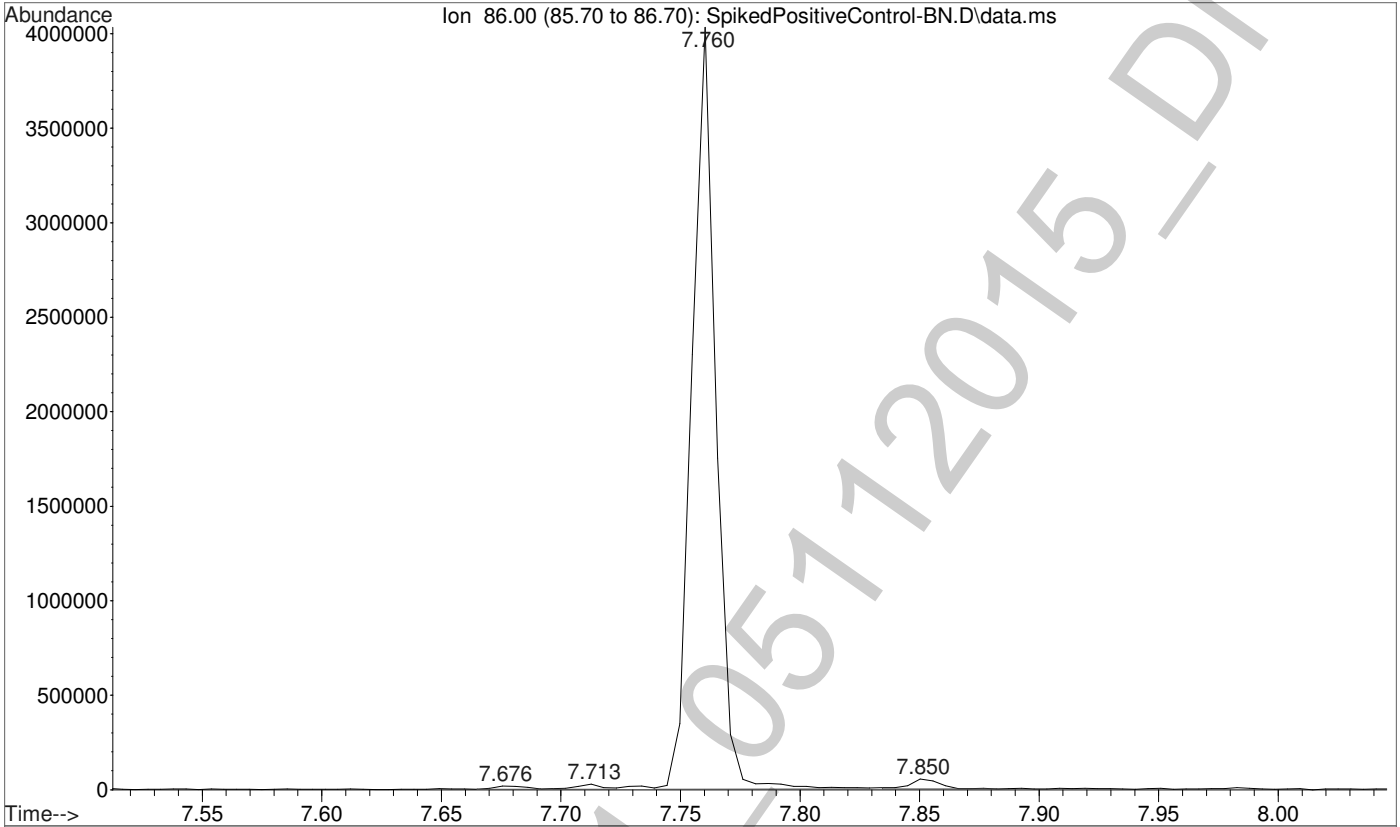



File :C:\gcms\1\data\Blood\051115BN\SpikedPositiveControl-BN.D
Operator : D Downey
Acquired : 11 May 2015 17:36 using AcqMethod BNSB120510.M
Instrument : Probie
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

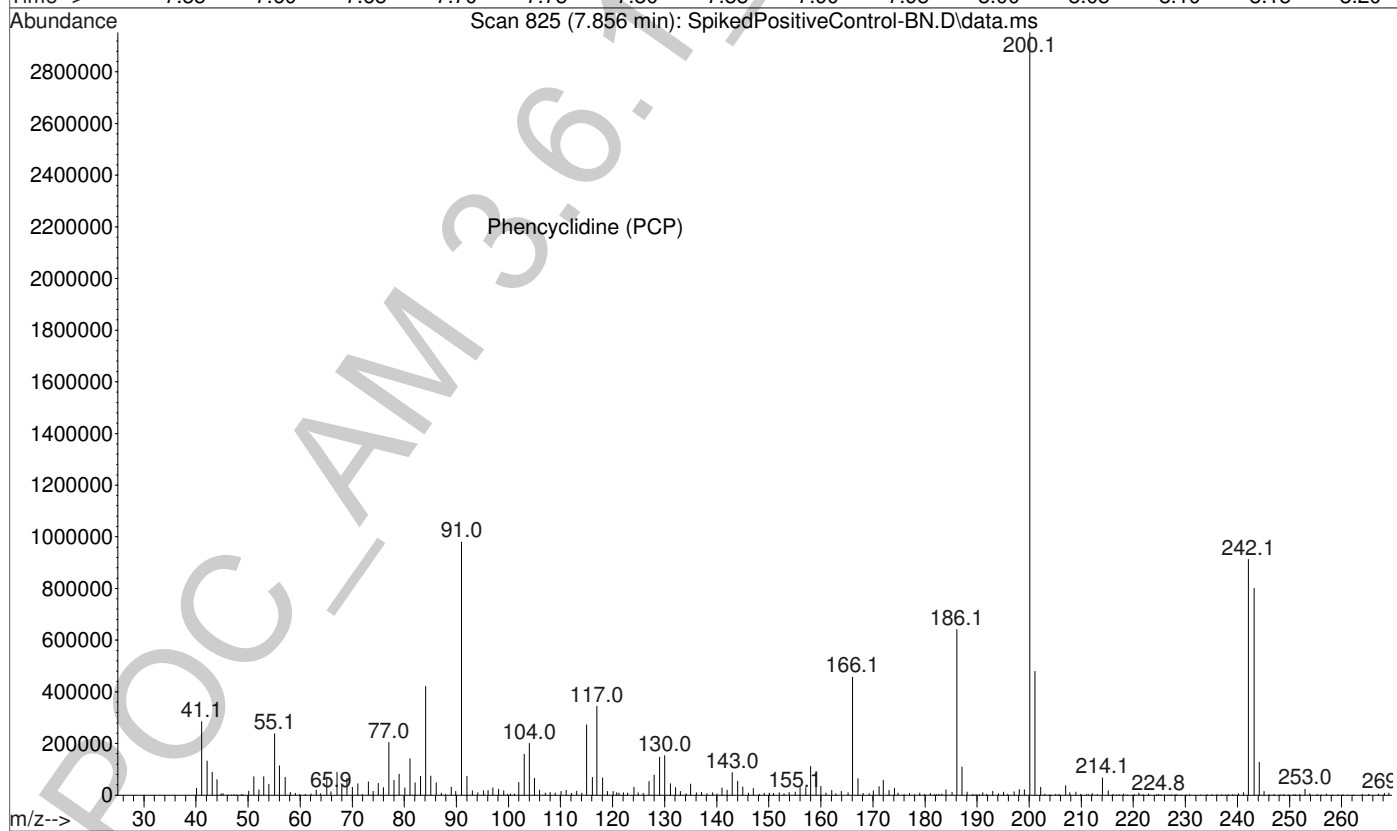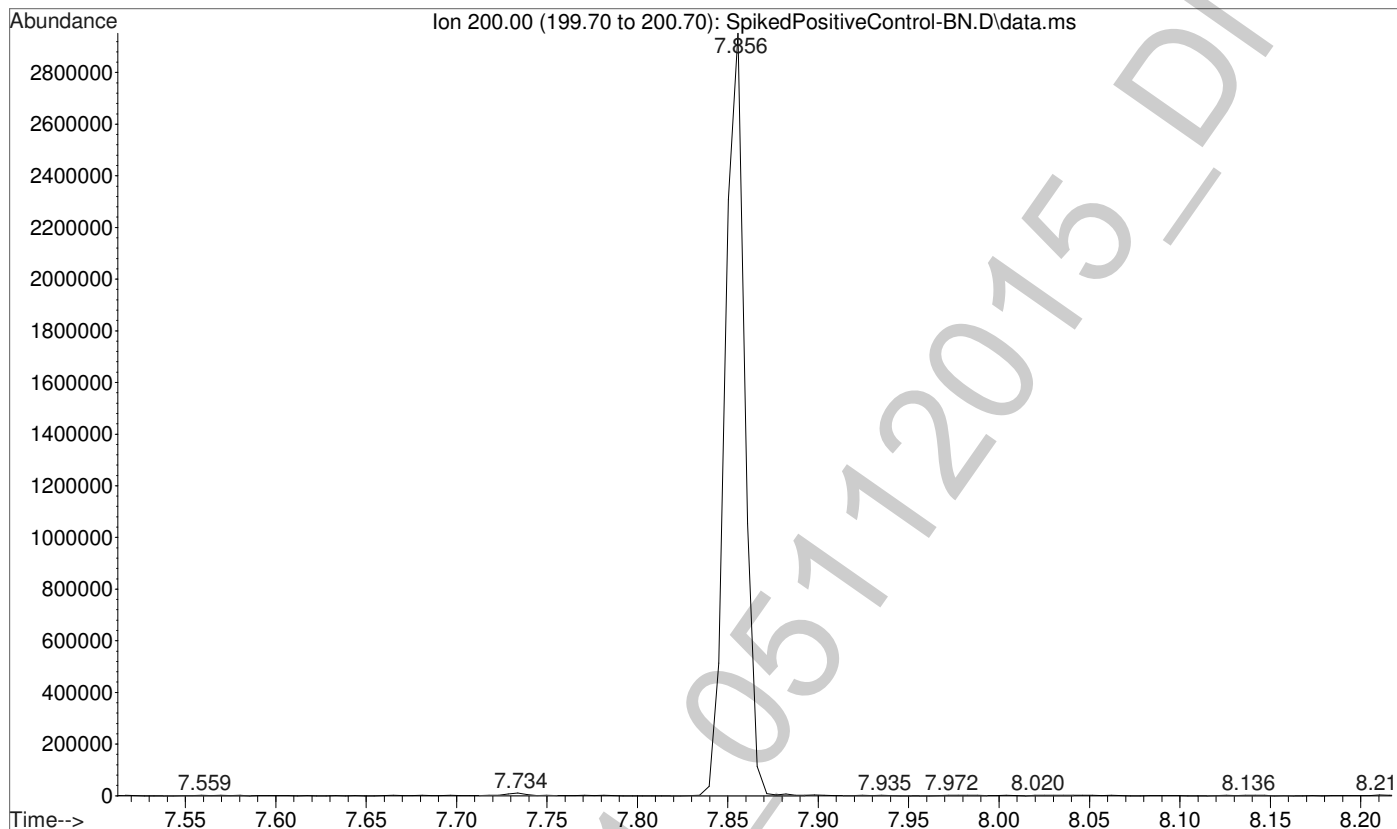



File :C:\gcms\1\data\Blood\051115BN\SpikedPositiveControl-BN.D
Operator : D Downey
Acquired : 11 May 2015 17:36 using AcqMethod BNSB120510.M
Instrument : Probie
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

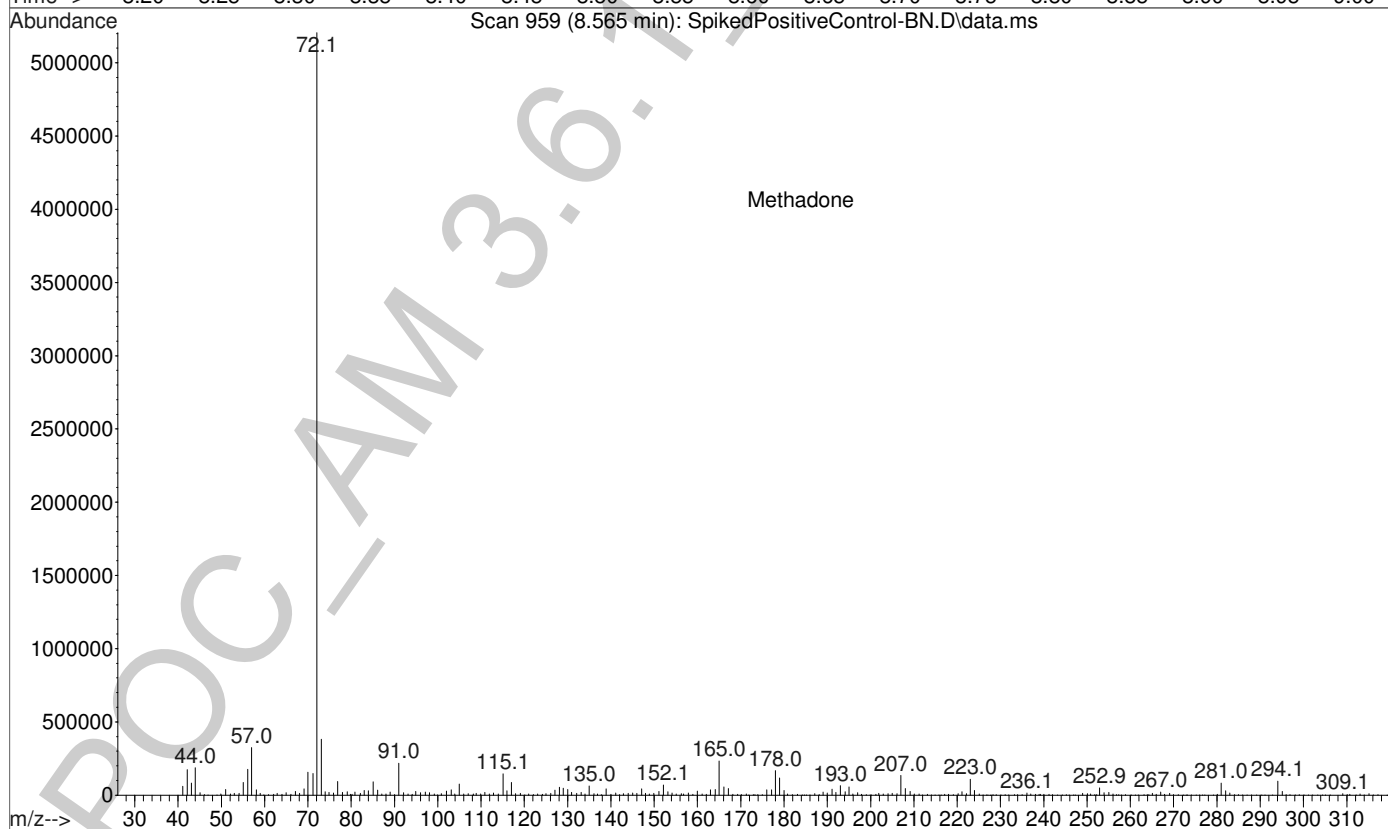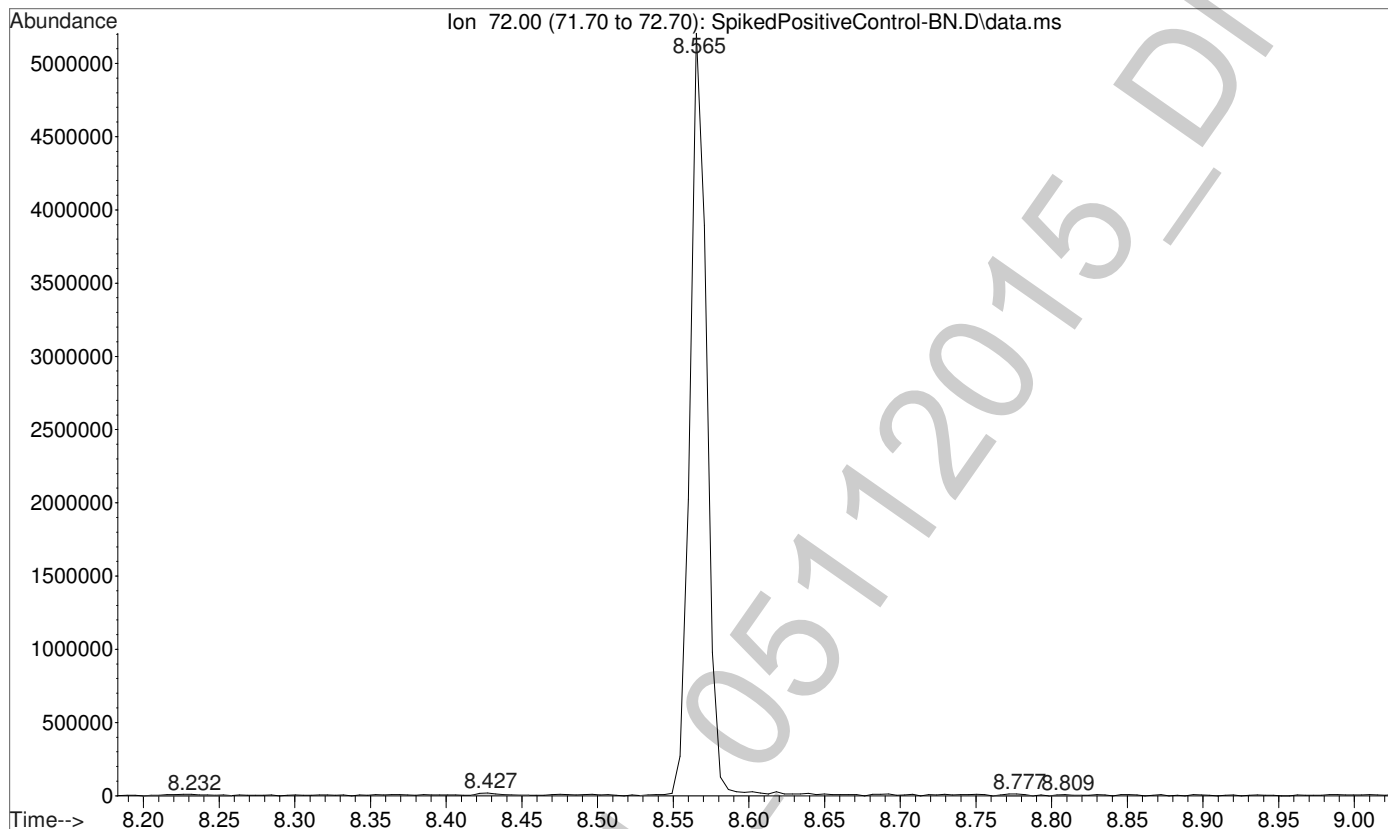



File :C:\gcms\1\data\Blood\051115BN\SpikedPositiveControl-BN.D
Operator : D Downey
Acquired : 11 May 2015 17:36 using AcqMethod BNSB120510.M
Instrument : Probie
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

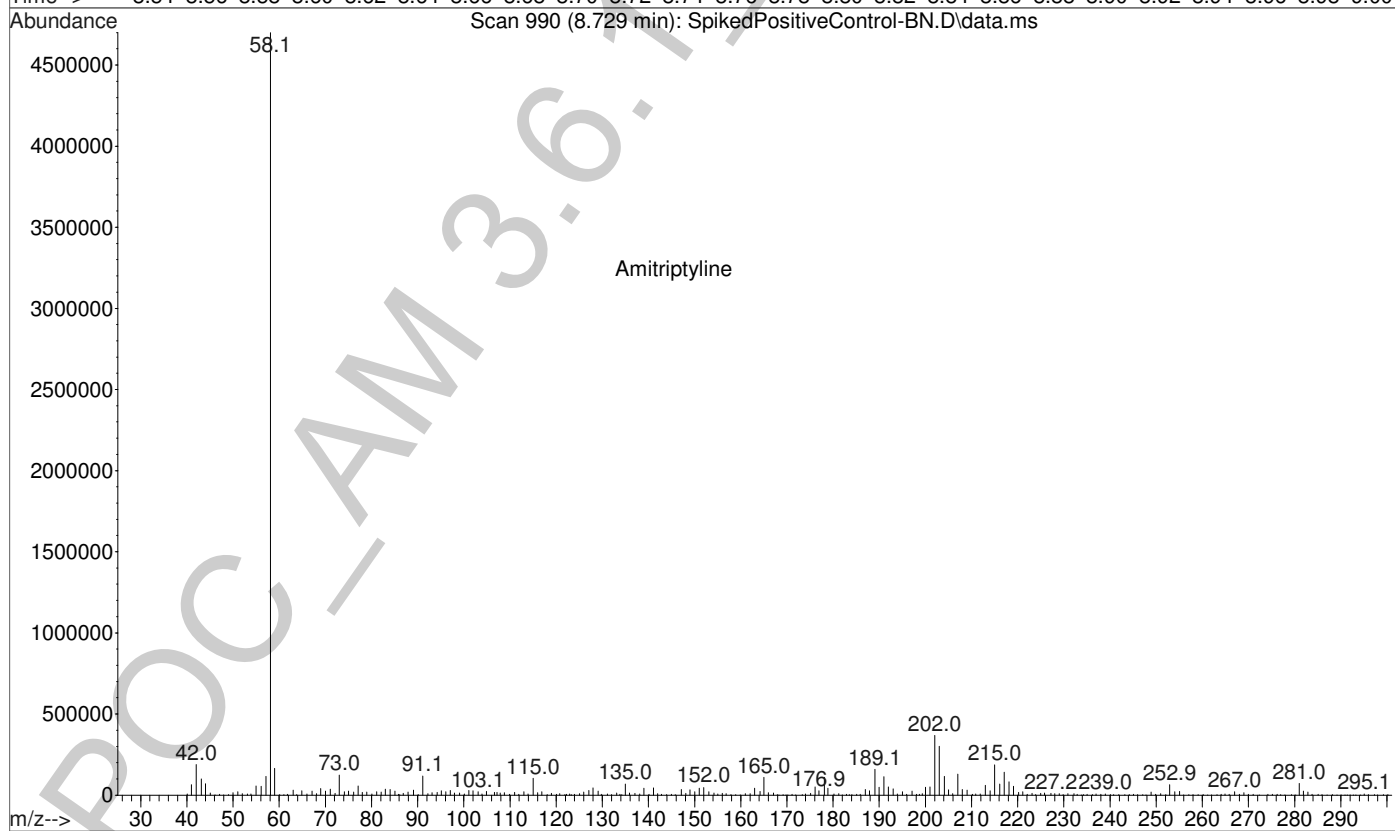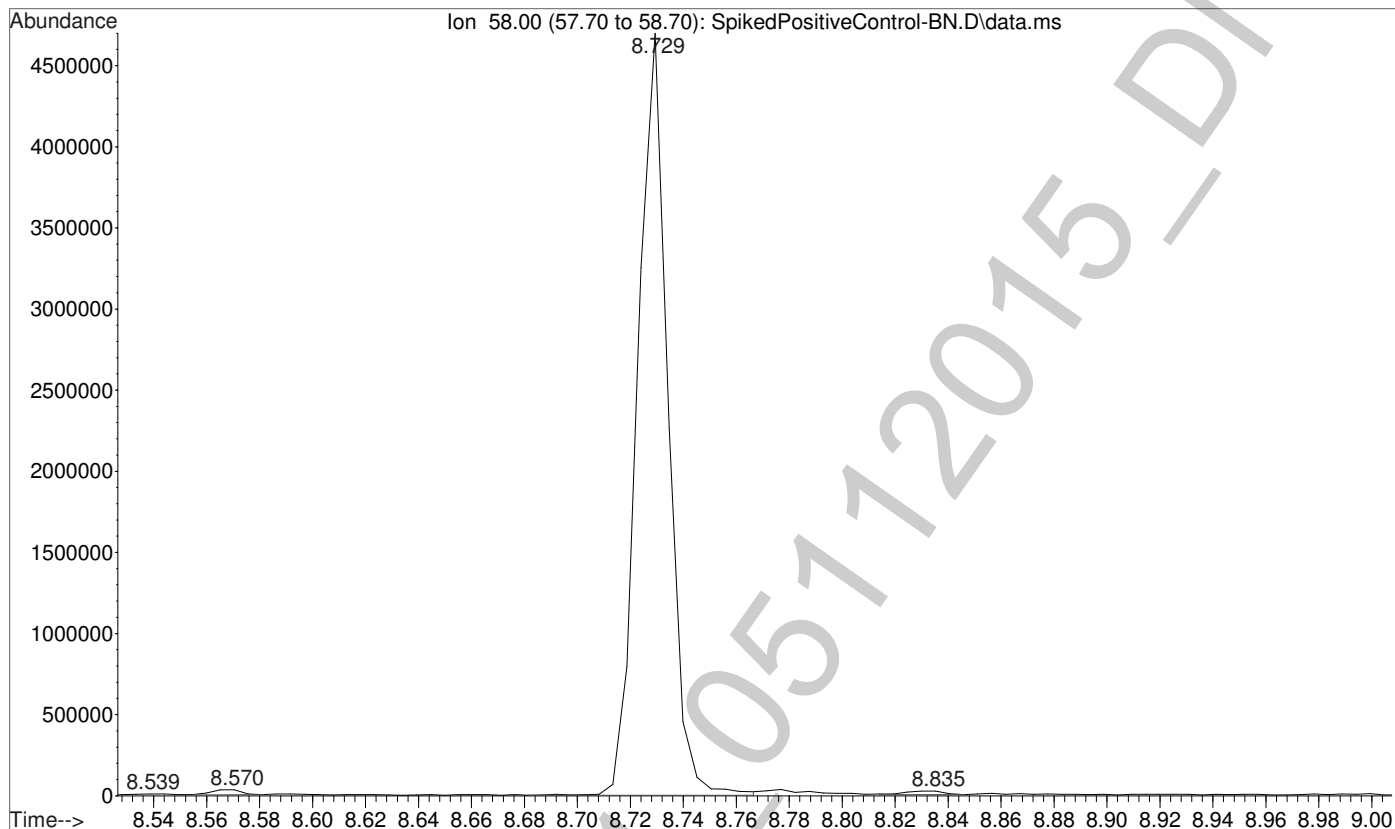



File :C:\gcms\1\data\Blood\051115BN\SpikedPositiveControl-BN.D
Operator : D Downey
Acquired : 11 May 2015 17:36 using AcqMethod BNSB120510.M
Instrument : Probie
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

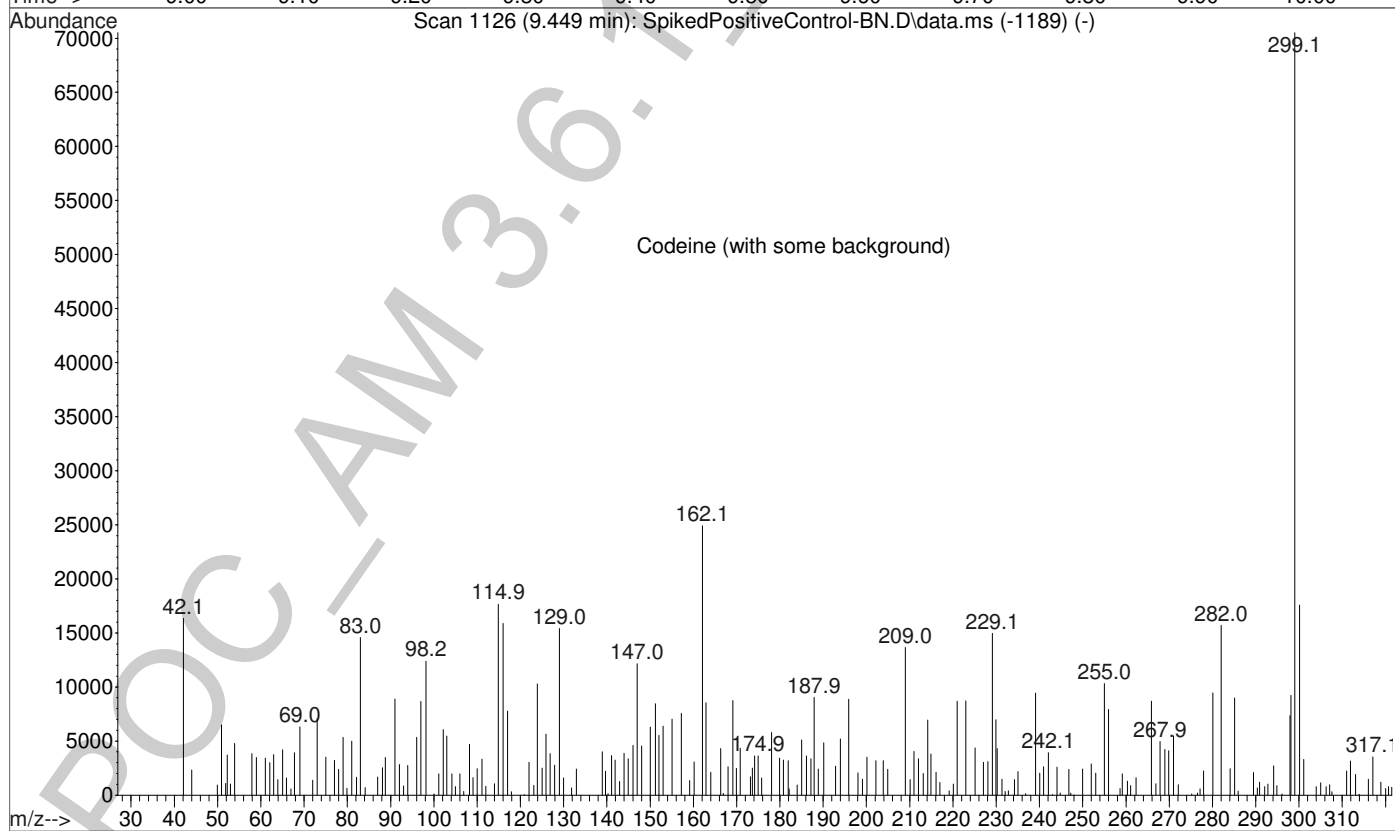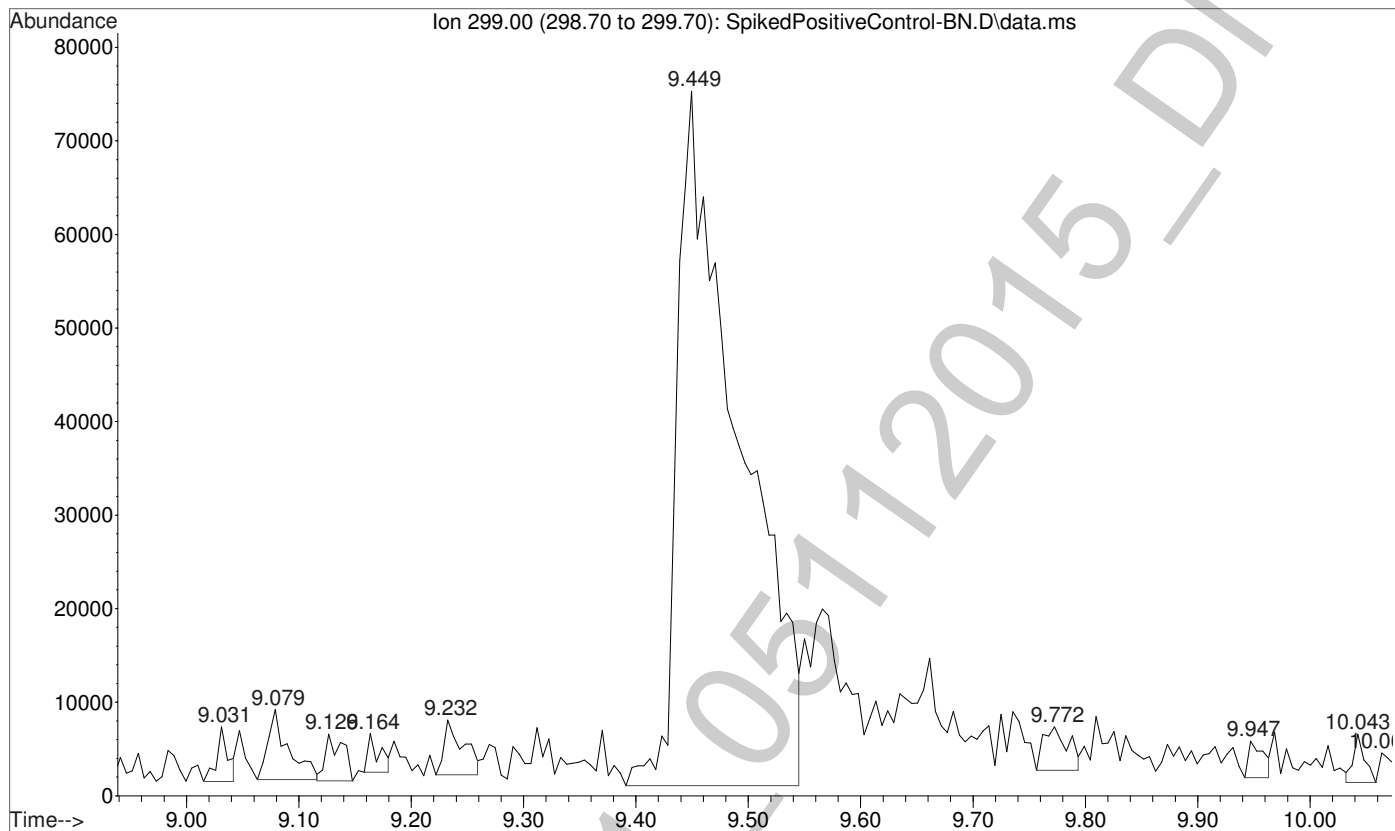

File :C:\gcms\1\data\Blood\051115BN\SpikedPositiveControl-BN.D
Operator : D Downey
Acquired : 11 May 2015 17:36 using AcqMethod BNSB120510.M
Instrument : Probie
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

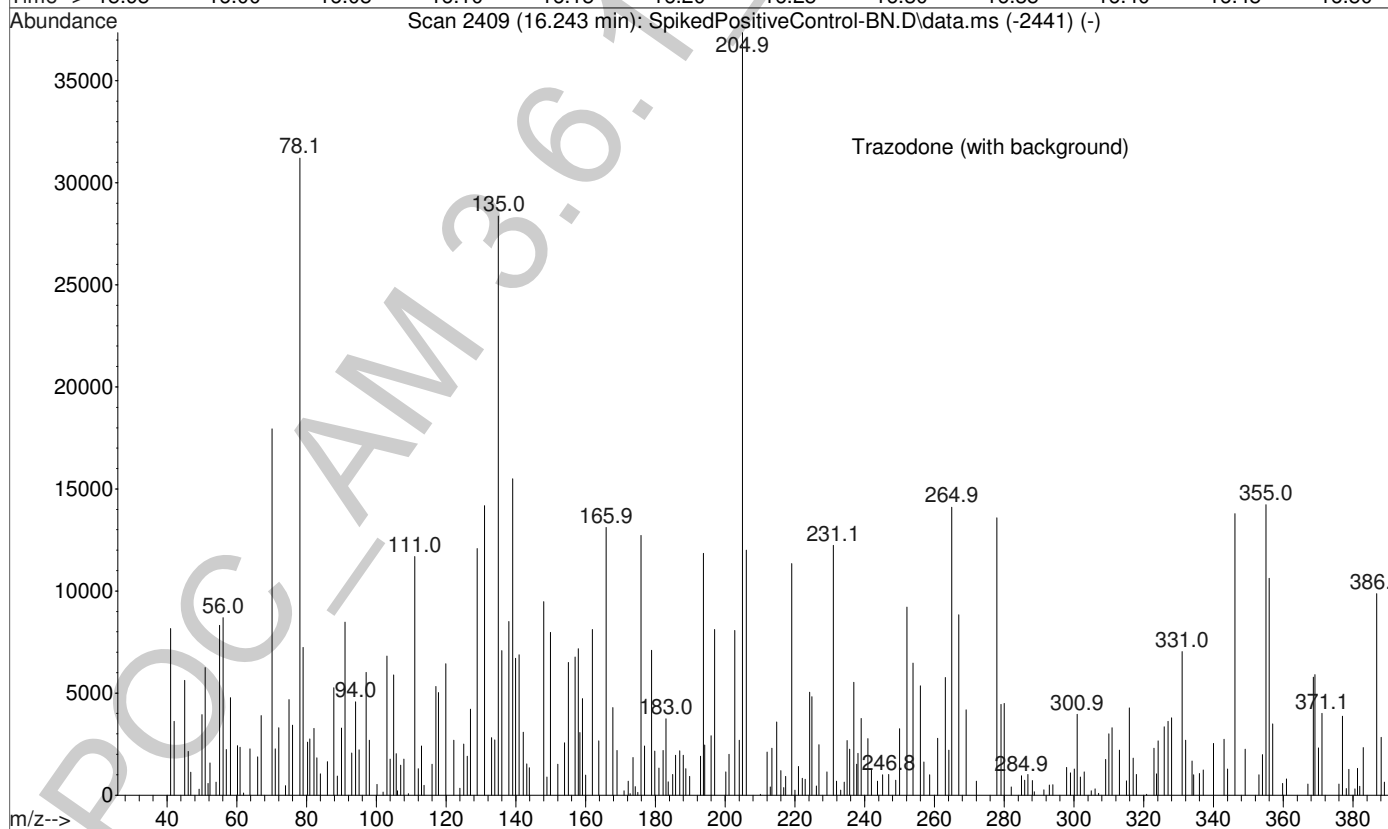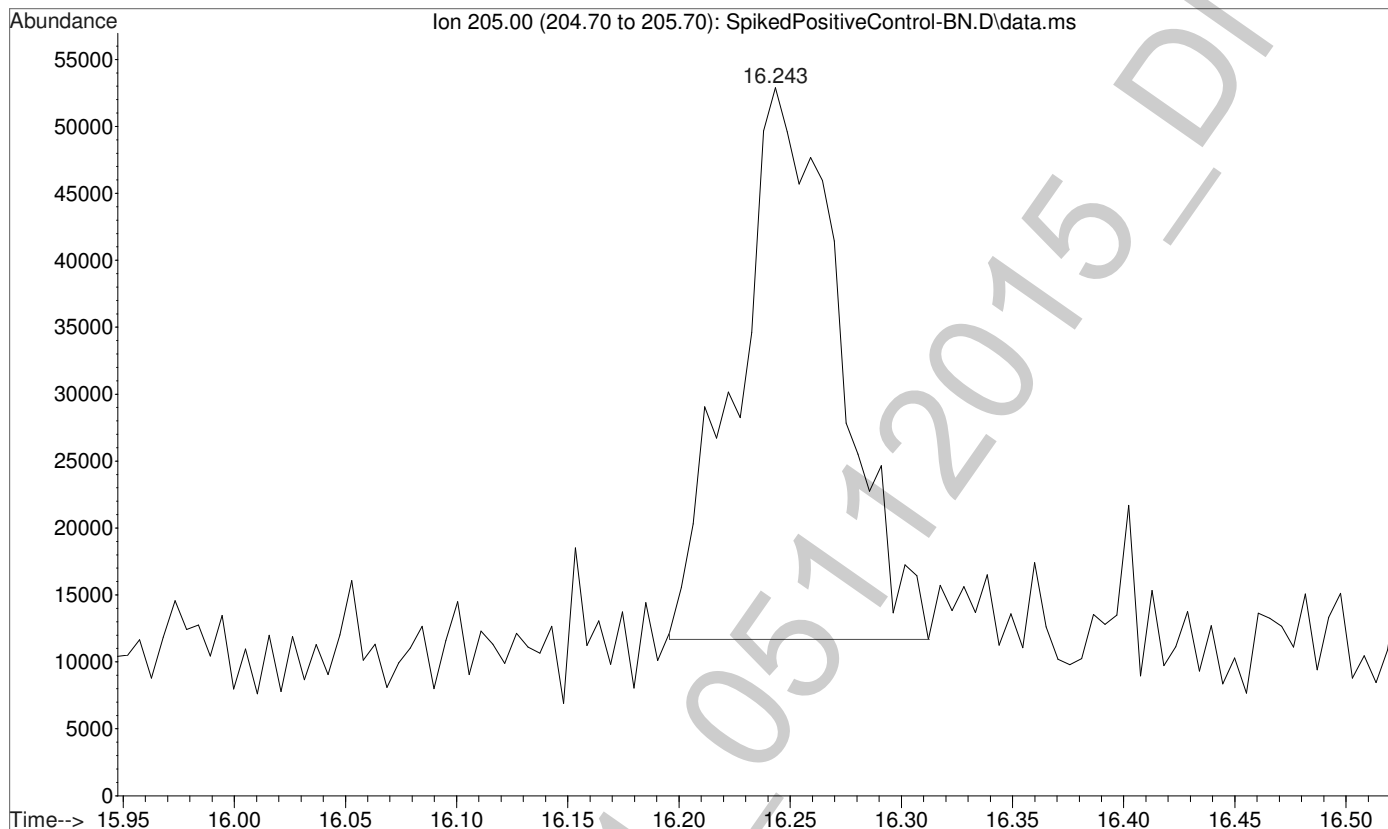

File :C:\gcms\1\data\Blood\051115BN\prbLK2.D
Operator : D Downey
Acquired : 11 May 2015 17:59 using AcqMethod BNSB120510.M
Instrument : Probie
Sample Name: Solvent Blank
Misc Info : Chloroform
Vial Number: 99

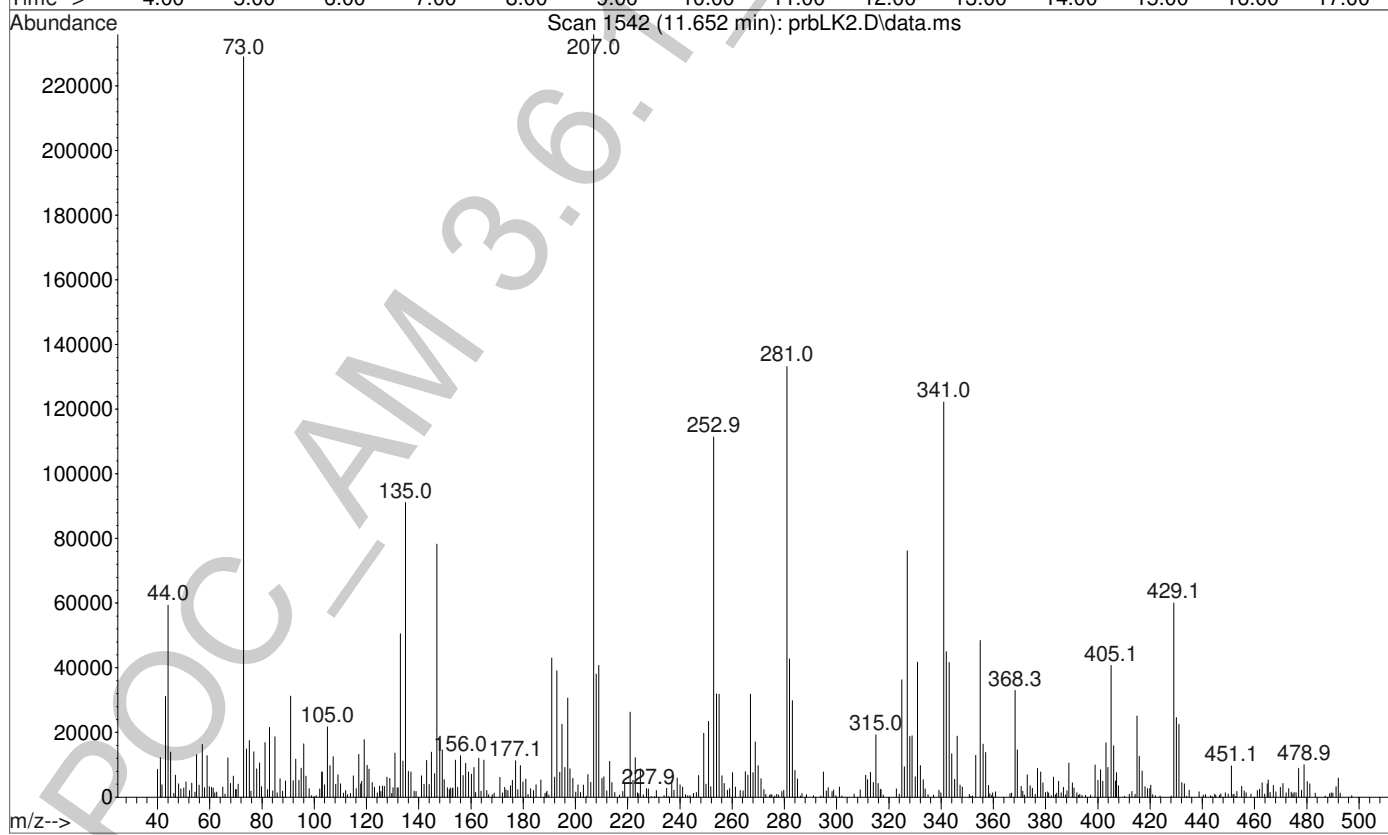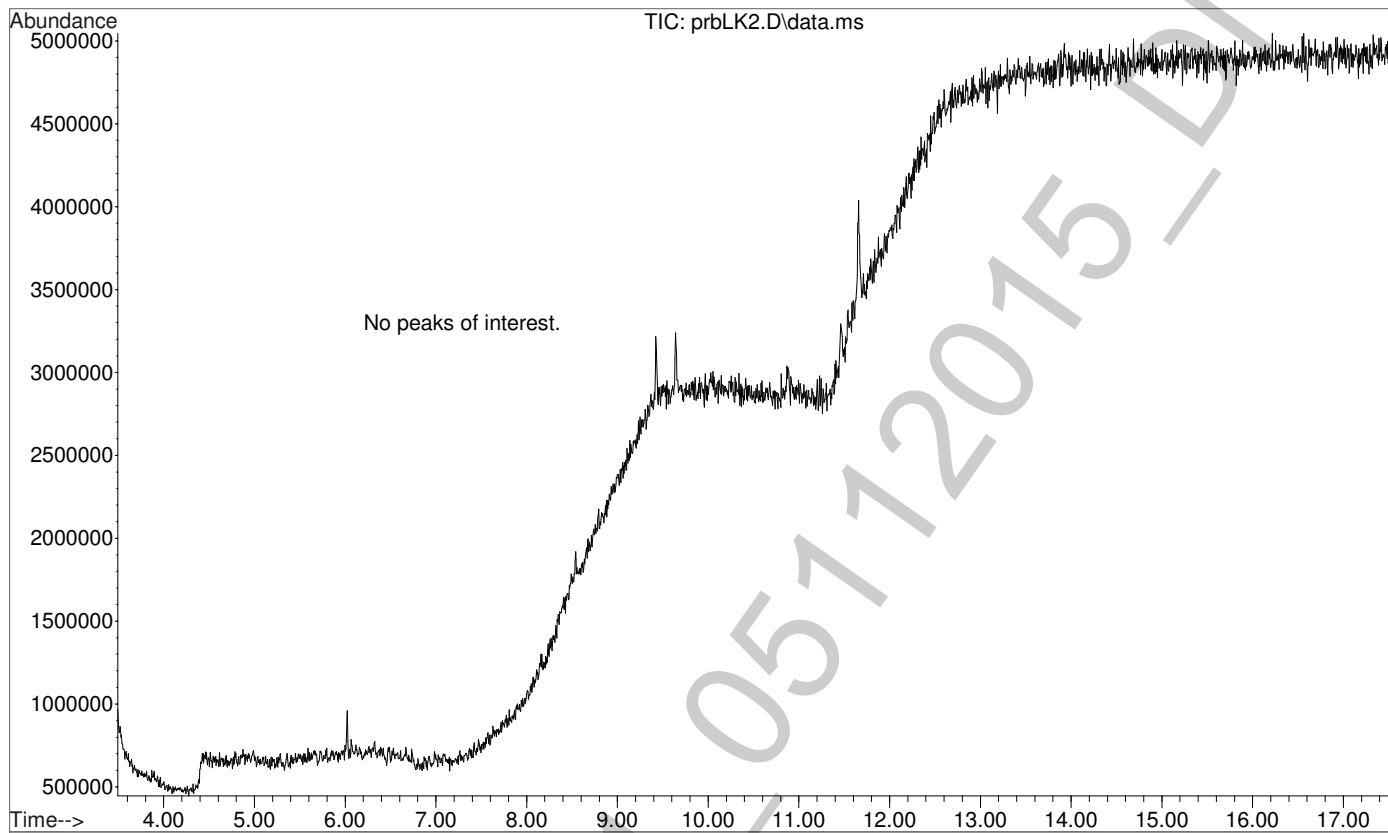

Analytical Method 3.6.1 & 3.6.7 QA Check List

Run Start Date: 05/11/15

Analyst: DND

(Long GC/MS temperature program)

Positive Control Compound List

- Methamphetamine
- Nicotine
- Meperidine
- Caffeine
- Diphenhydramine
- Lidocaine
- PCP
- Methadone
- Amitriptyline
- Codeine
- Trazodone



Internal Standards

- Benzphetamine
- Papaverine


Optional back extraction **not** performed.
Samples reconstituted in methanol.





File :C:\gcms\1\data\Blood\051115BN\Reinjection Longer GC Method\P
... rerun Solvent Blankr.D
Operator : D Downey
Instrument : Probie
Acquired : 11 May 2015 18:22 using AcqMethod GBT092509.M
Sample Name: Pre-run Solvent Blank
Misc Info : Chloroform

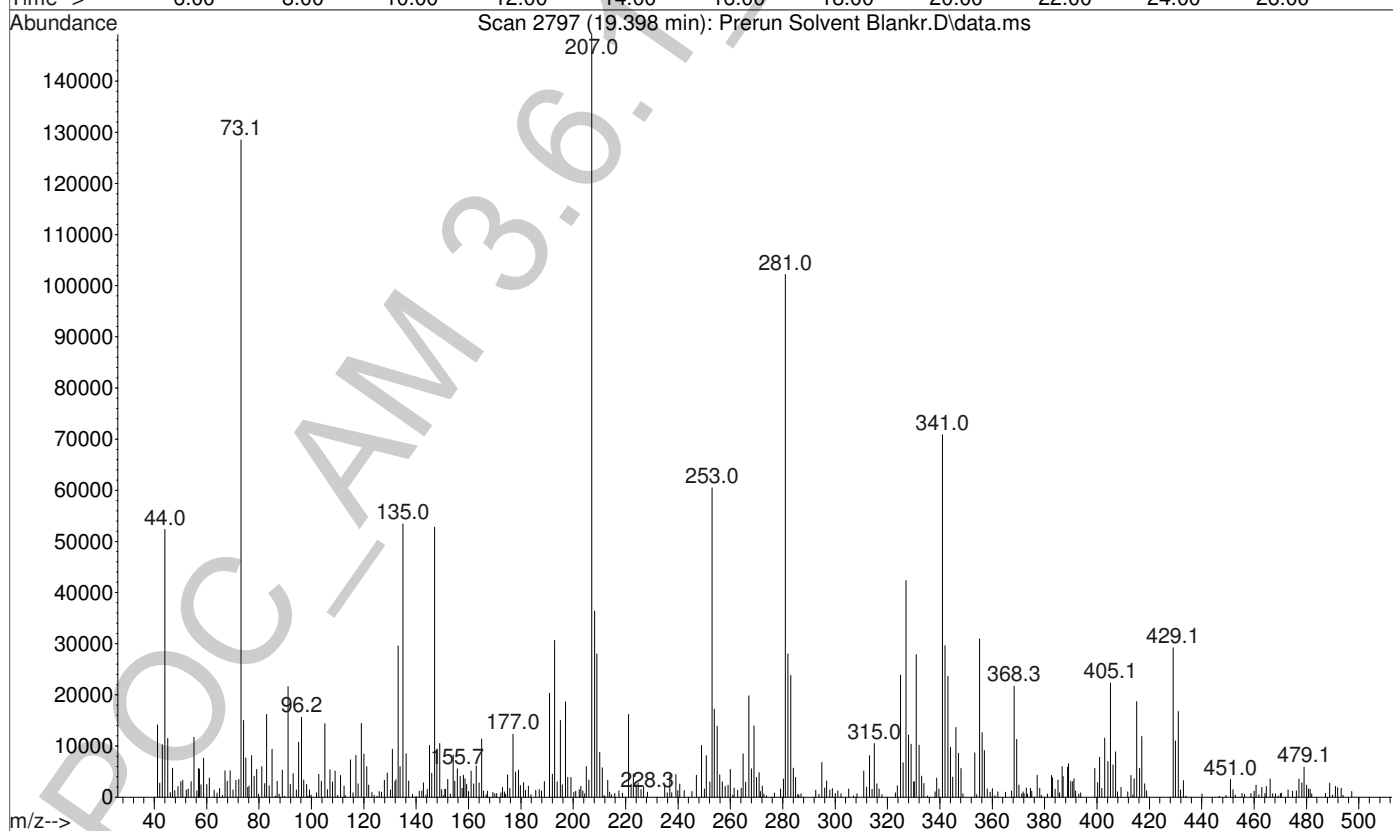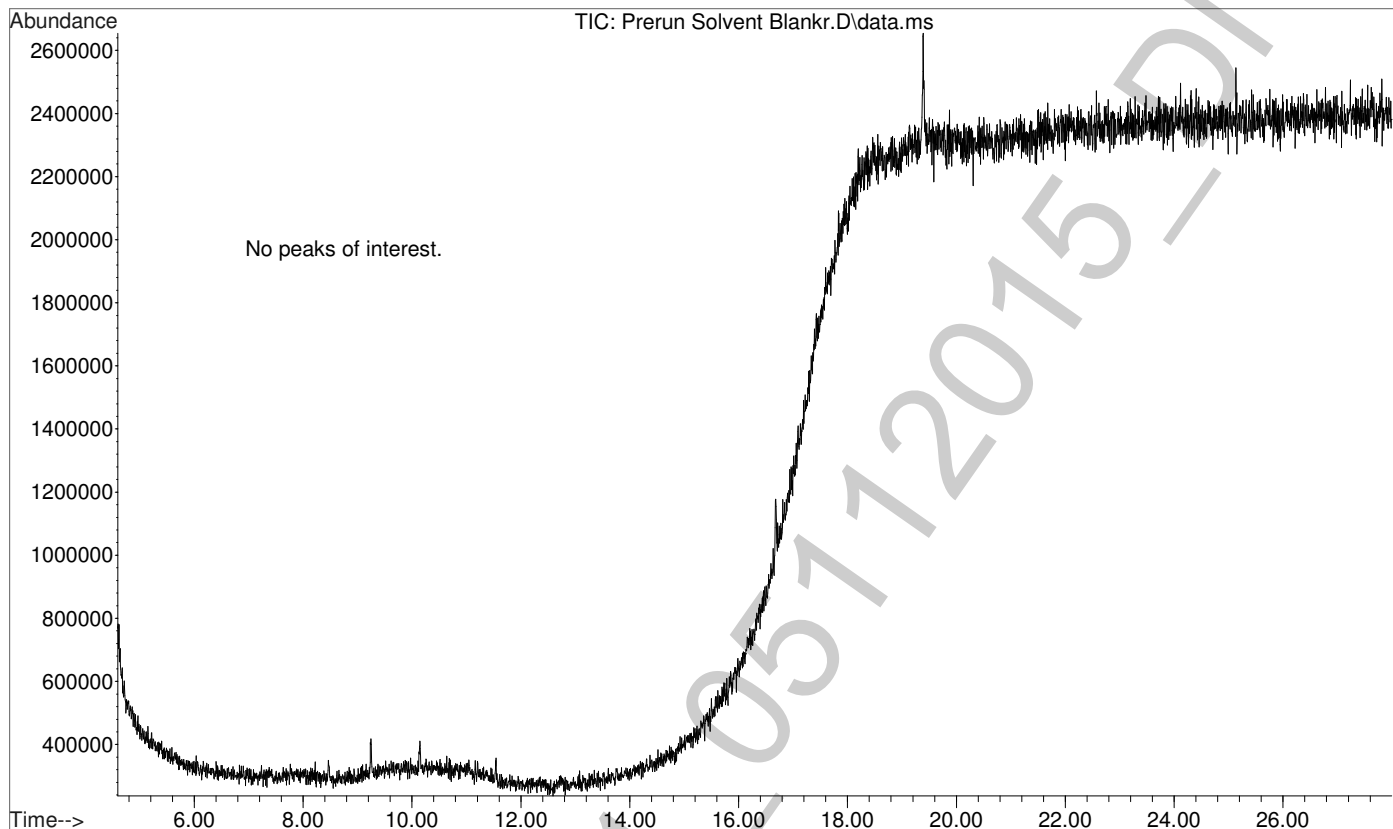



File :C:\gcms\1\data\Blood\051115BN\Reinjection Longer GC Method\N
... egativeControl-BNr.D
Operator : D Downey
Instrument : Probie
Acquired : 11 May 2015 18:56 using AcqMethod GBT092509.M
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1

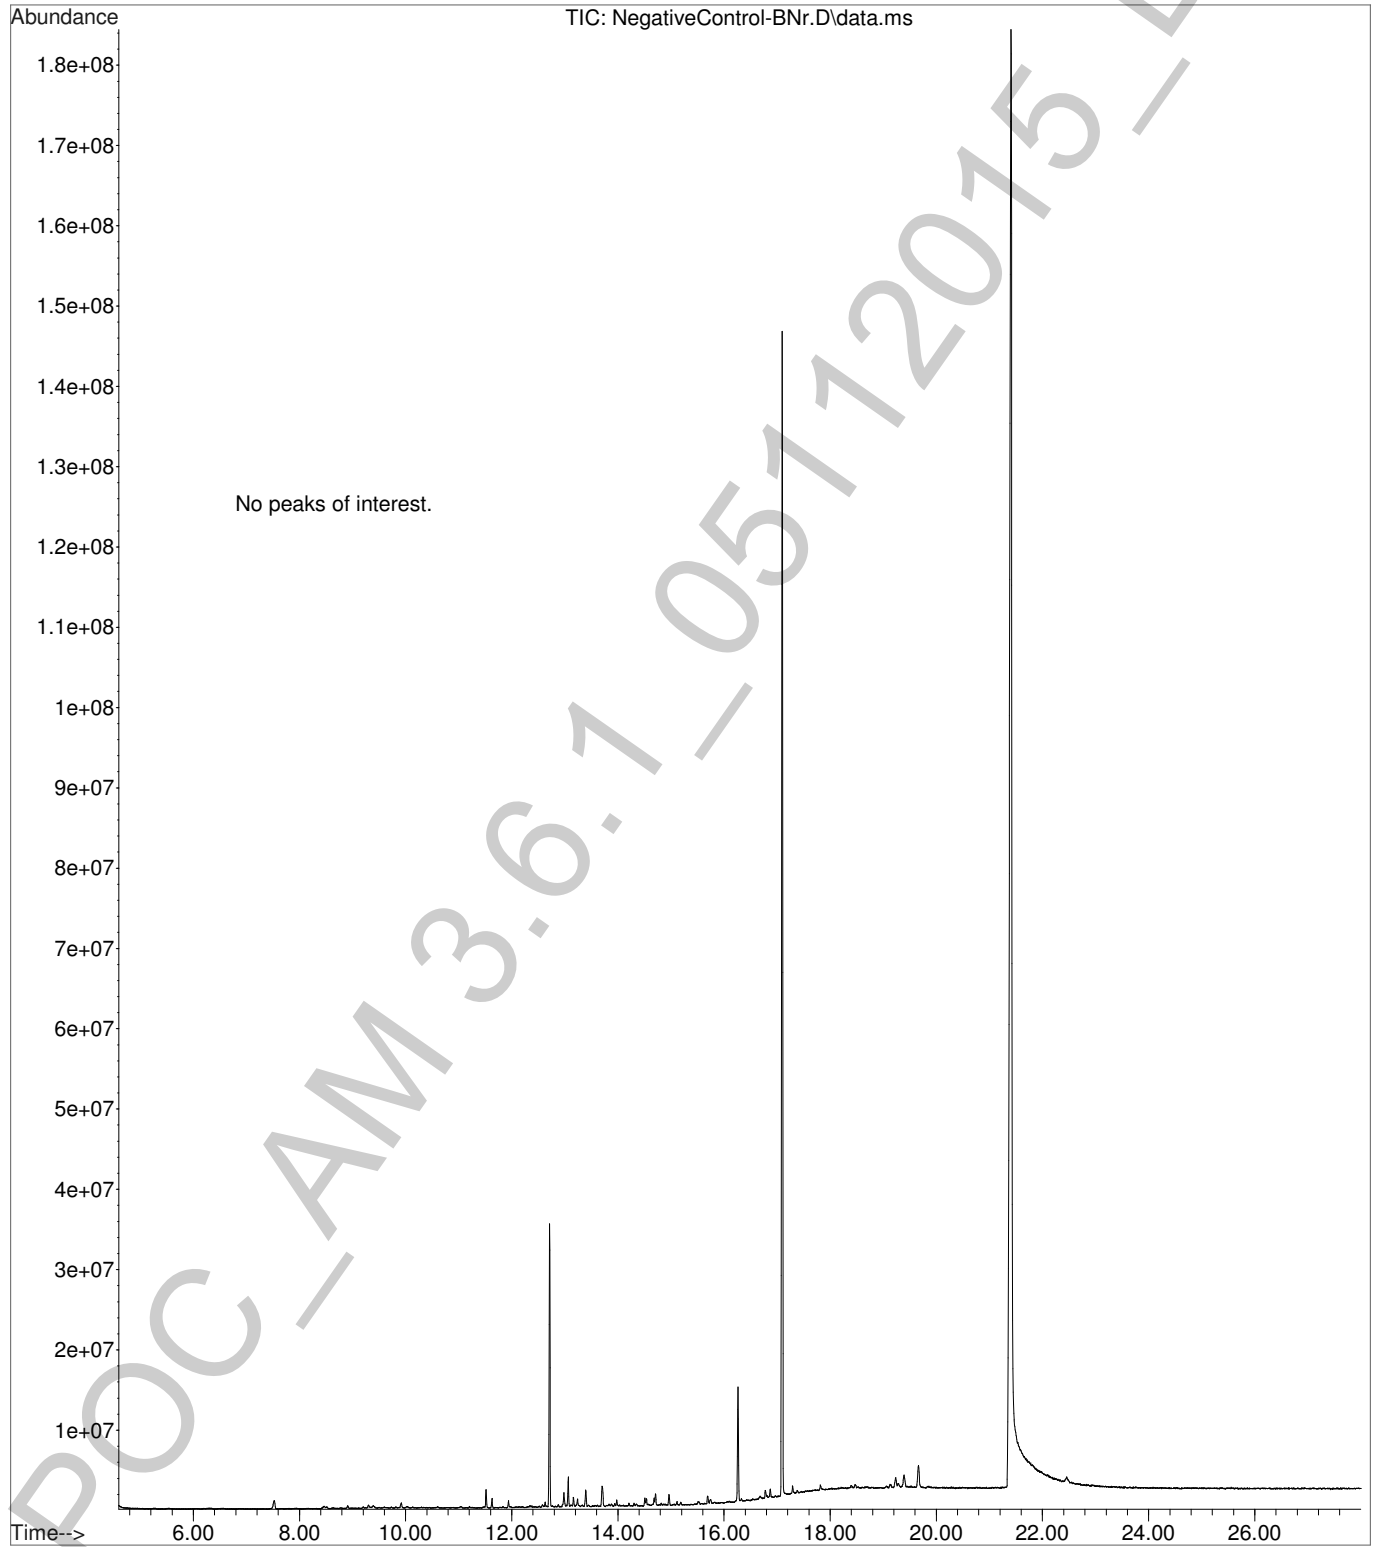


File :C:\gcms\1\data\Blood\051115BN\Reinjection Longer GC Method\N
... egativeControl-BNr.D
Operator : D Downey
Instrument : Probie
Acquired : 11 May 2015 18:56 using AcqMethod GBT092509.M
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1

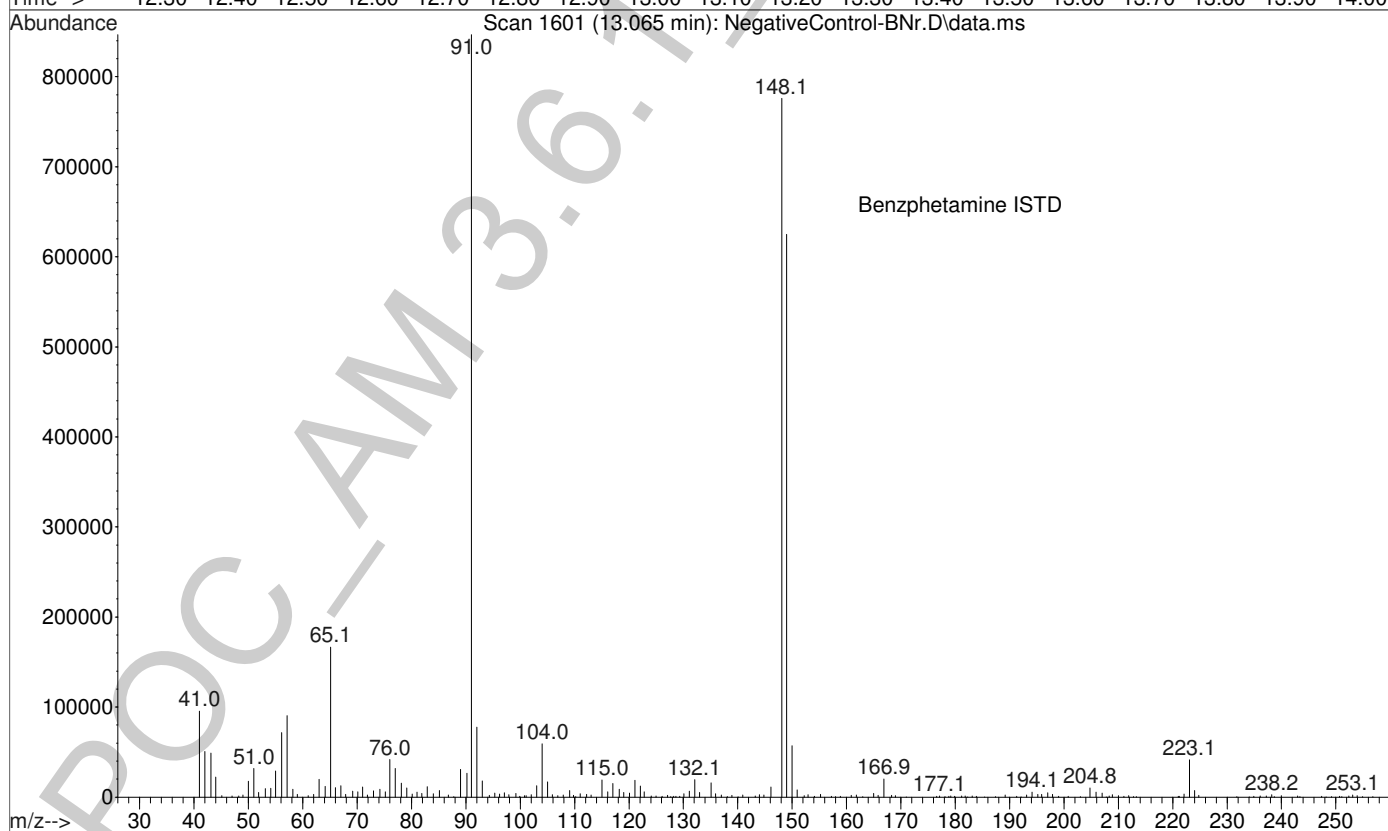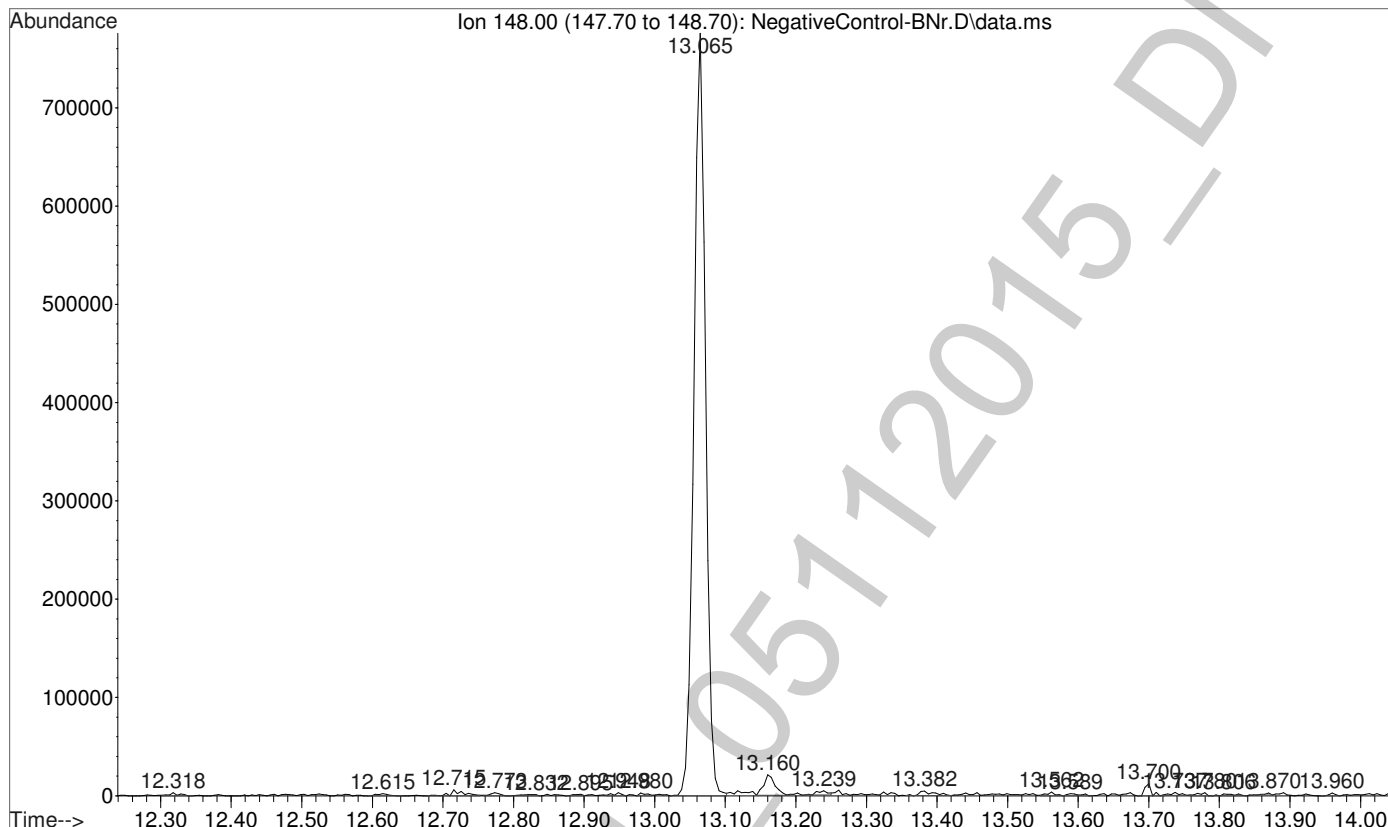



File :C:\gcms\1\data\Blood\051115BN\Reinjection Longer GC Method\N
... egativeControl-BNr.D
Operator : D Downey
Instrument : Probie
Acquired : 11 May 2015 18:56 using AcqMethod GBT092509.M
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1

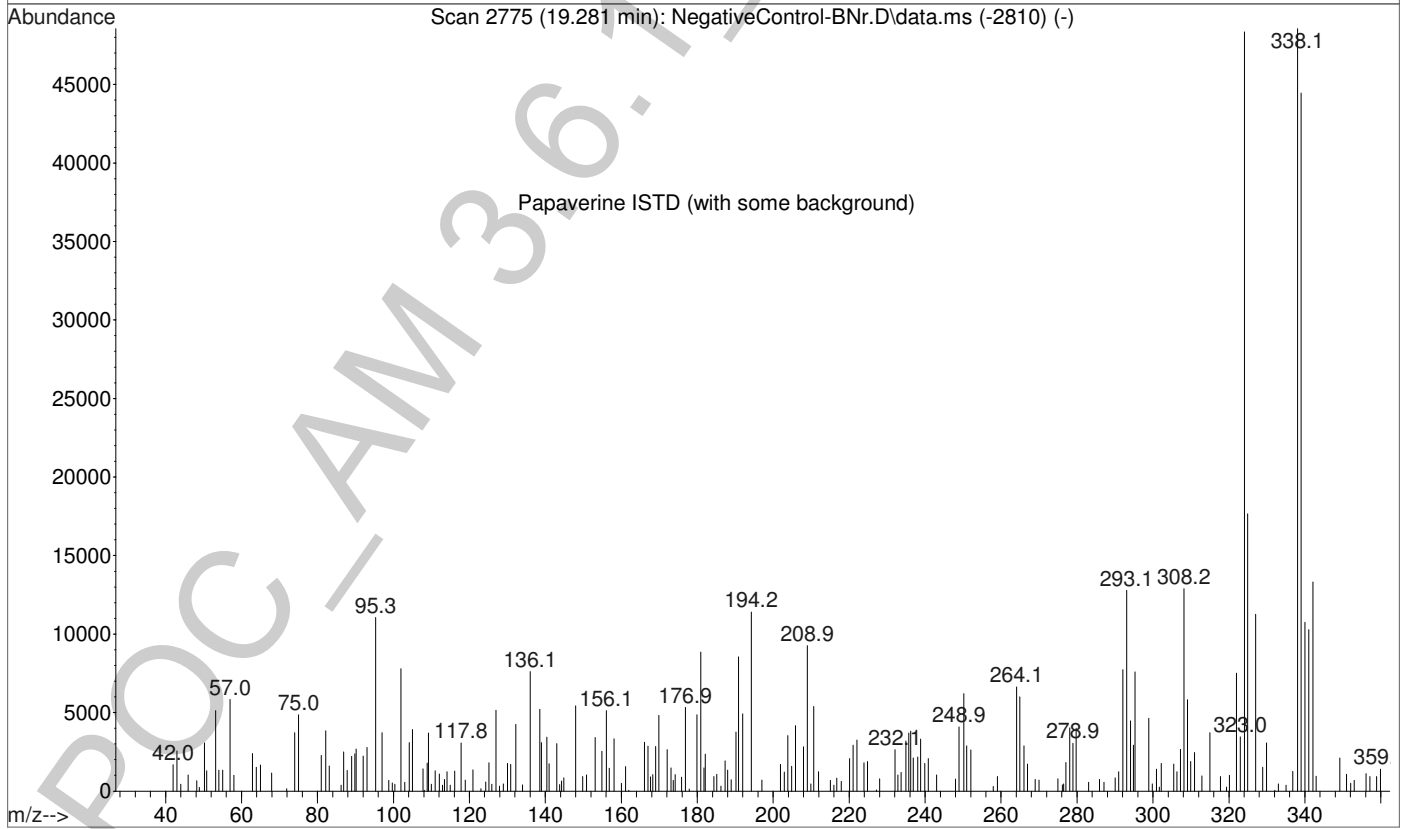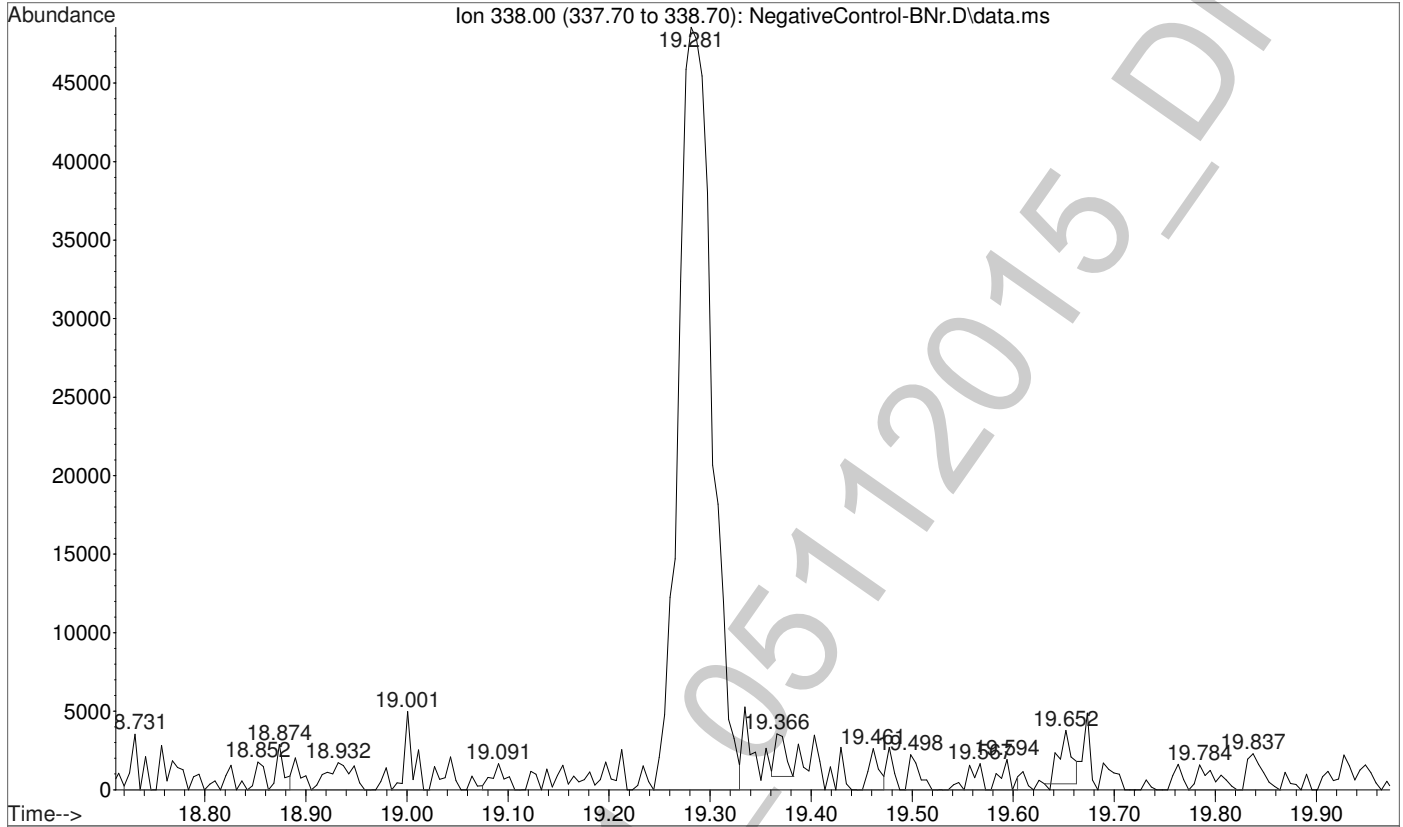



File :C:\gcms\1\data\Blood\051115BN\Reinjection Longer GC Method\S
... pikedPositiveControl-BNr.D
Operator : D Downey
Instrument : Probie
Acquired : 11 May 2015 19:30 using AcqMethod GBT092509.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

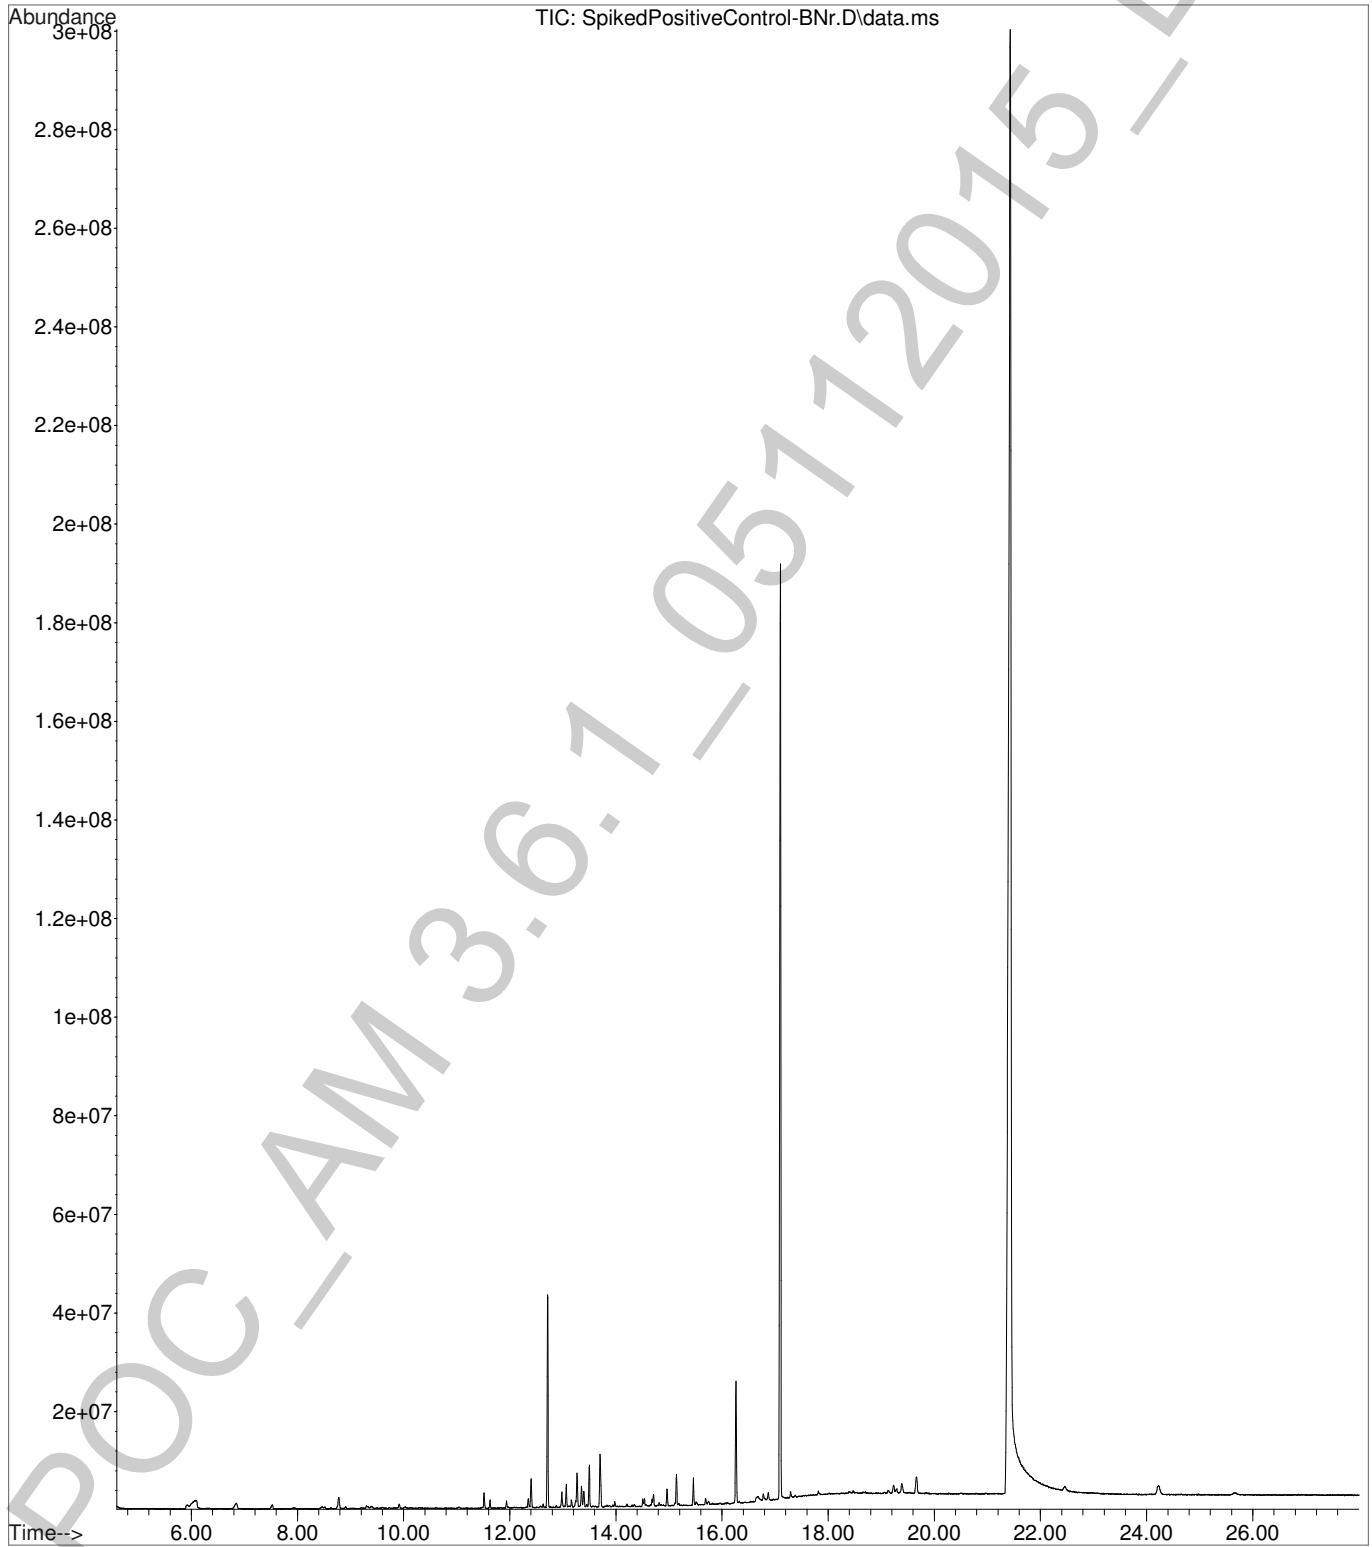



File :C:\gcms\1\data\Blood\051115BN\Reinjection Longer GC Method\S
... pikedPositiveControl-BNr.D
Operator : D Downey
Instrument : Probie
Acquired : 11 May 2015 19:30 using AcqMethod GBT092509.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

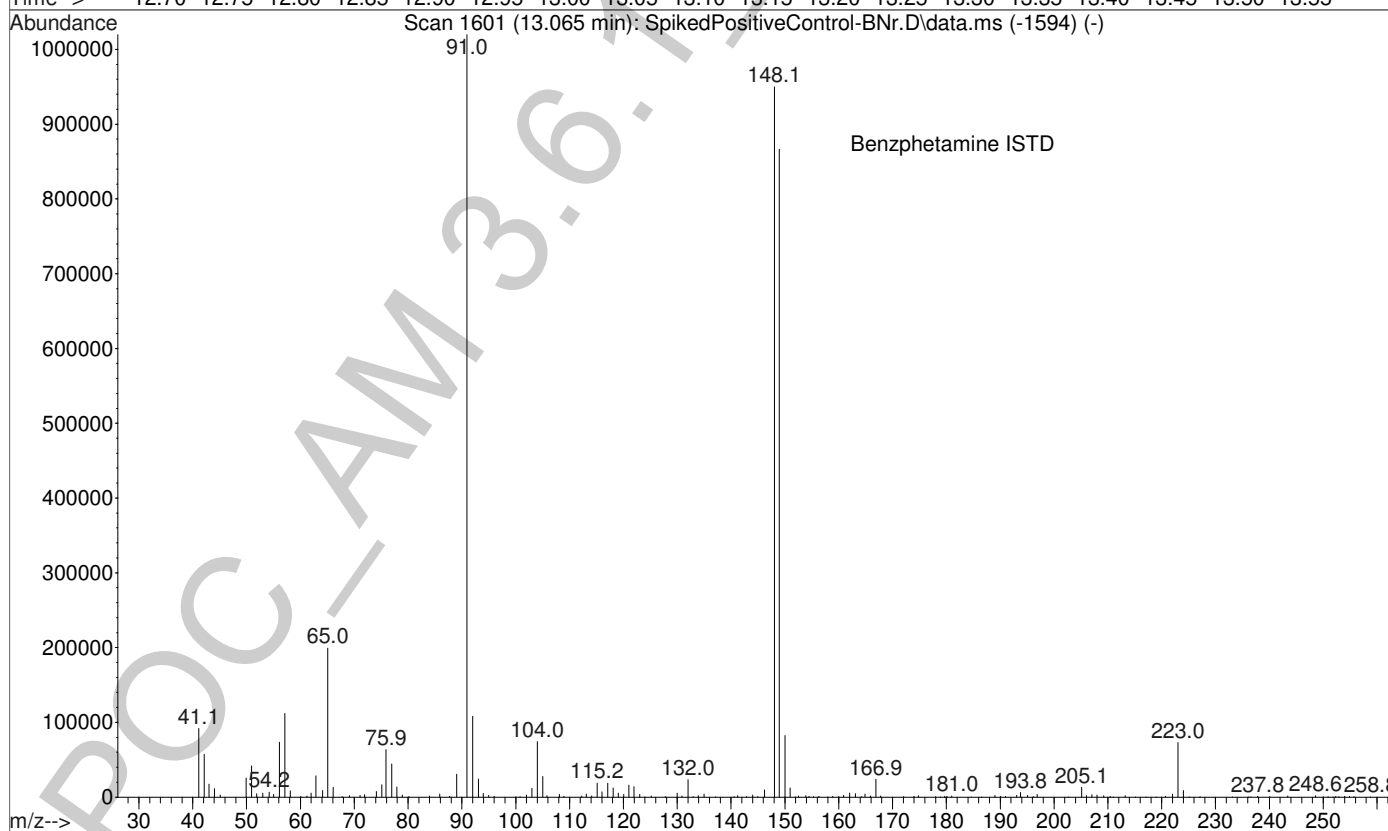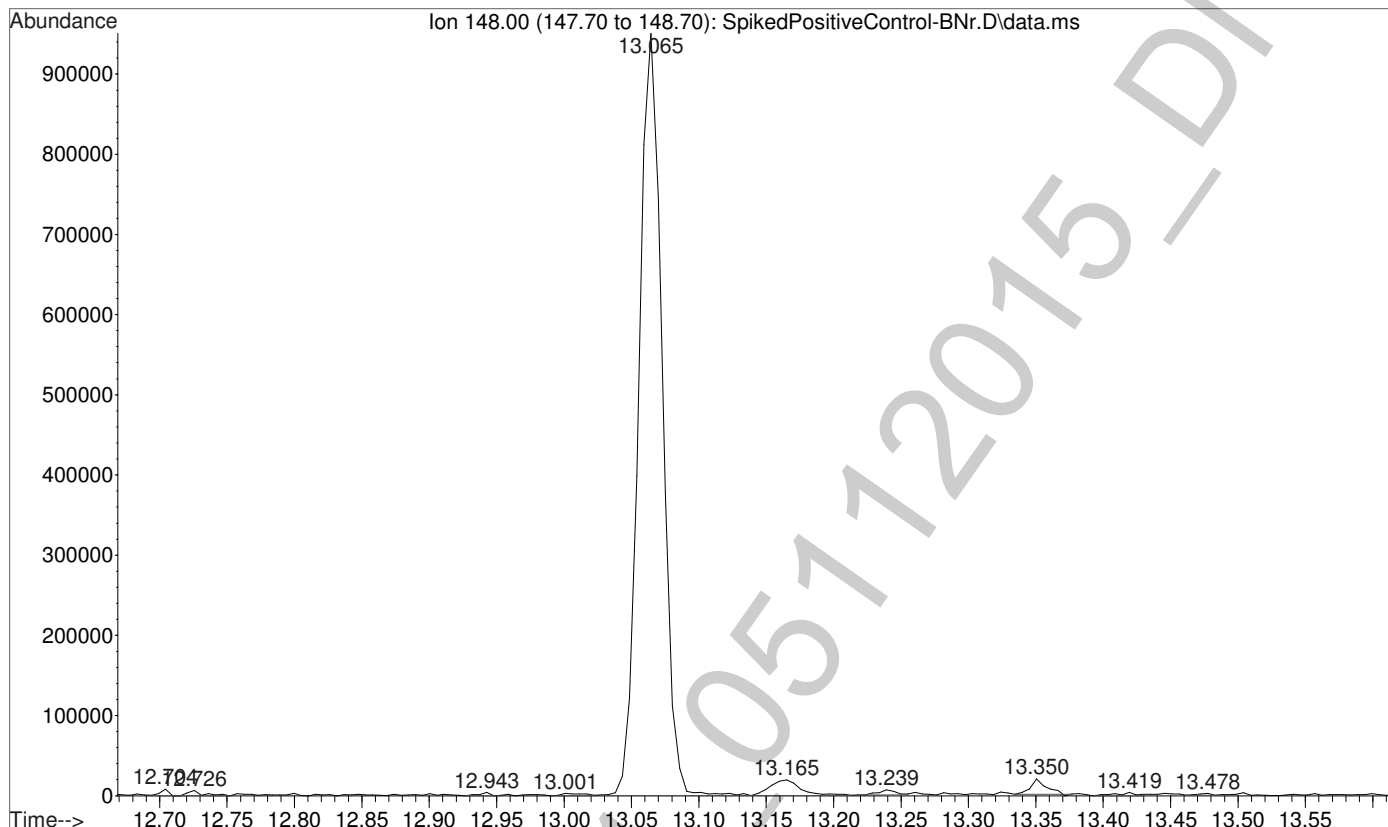



File :C:\gcms\1\data\Blood\051115BN\Reinjection Longer GC Method\S
... pikedPositiveControl-BNr.D
Operator : D Downey
Instrument : Probie
Acquired : 11 May 2015 19:30 using AcqMethod GBT092509.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

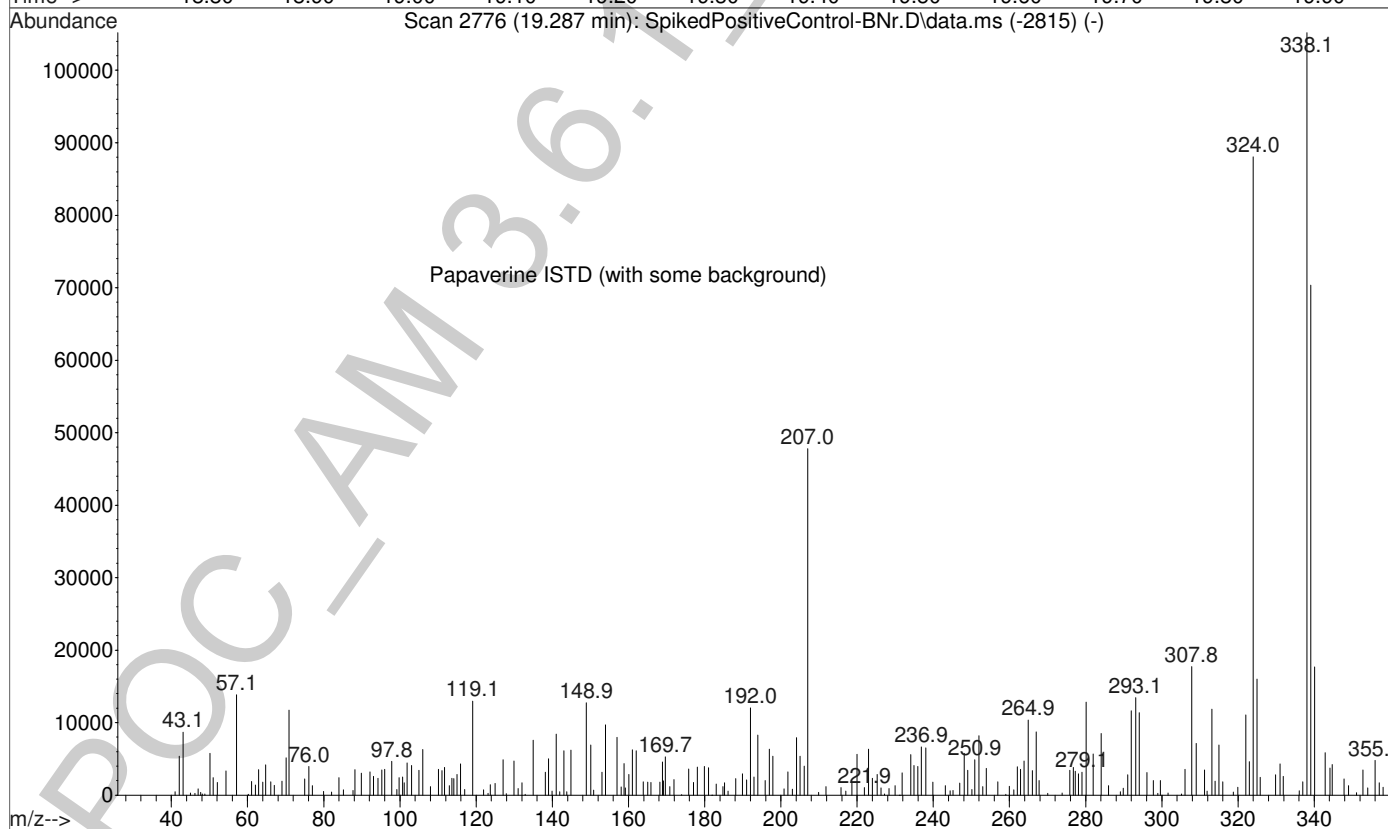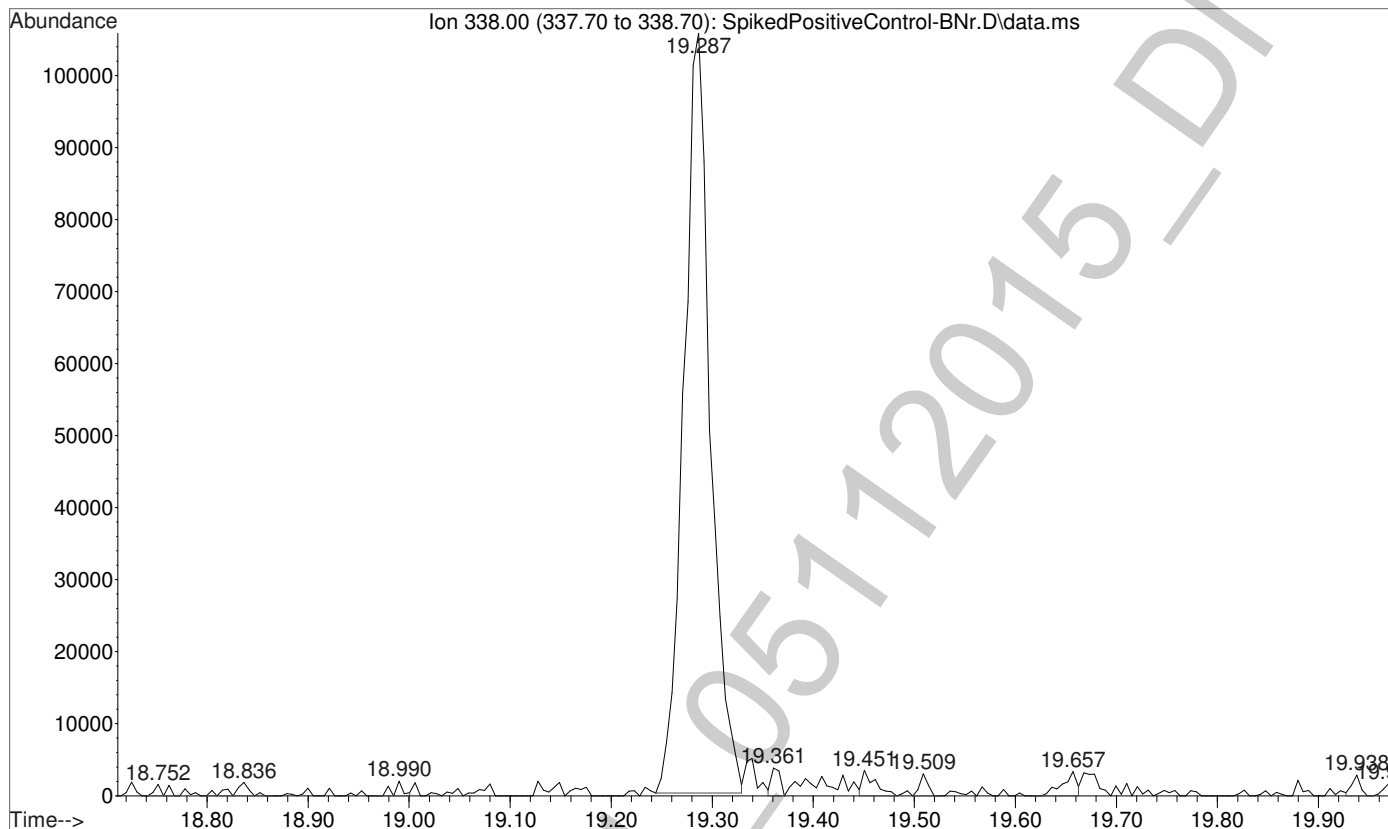



File :C:\gcms\1\data\Blood\051115BN\Reinjection Longer GC Method\S
... pikedPositiveControl-BNr.D
Operator : D Downey
Instrument : Probie
Acquired : 11 May 2015 19:30 using AcqMethod GBT092509.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

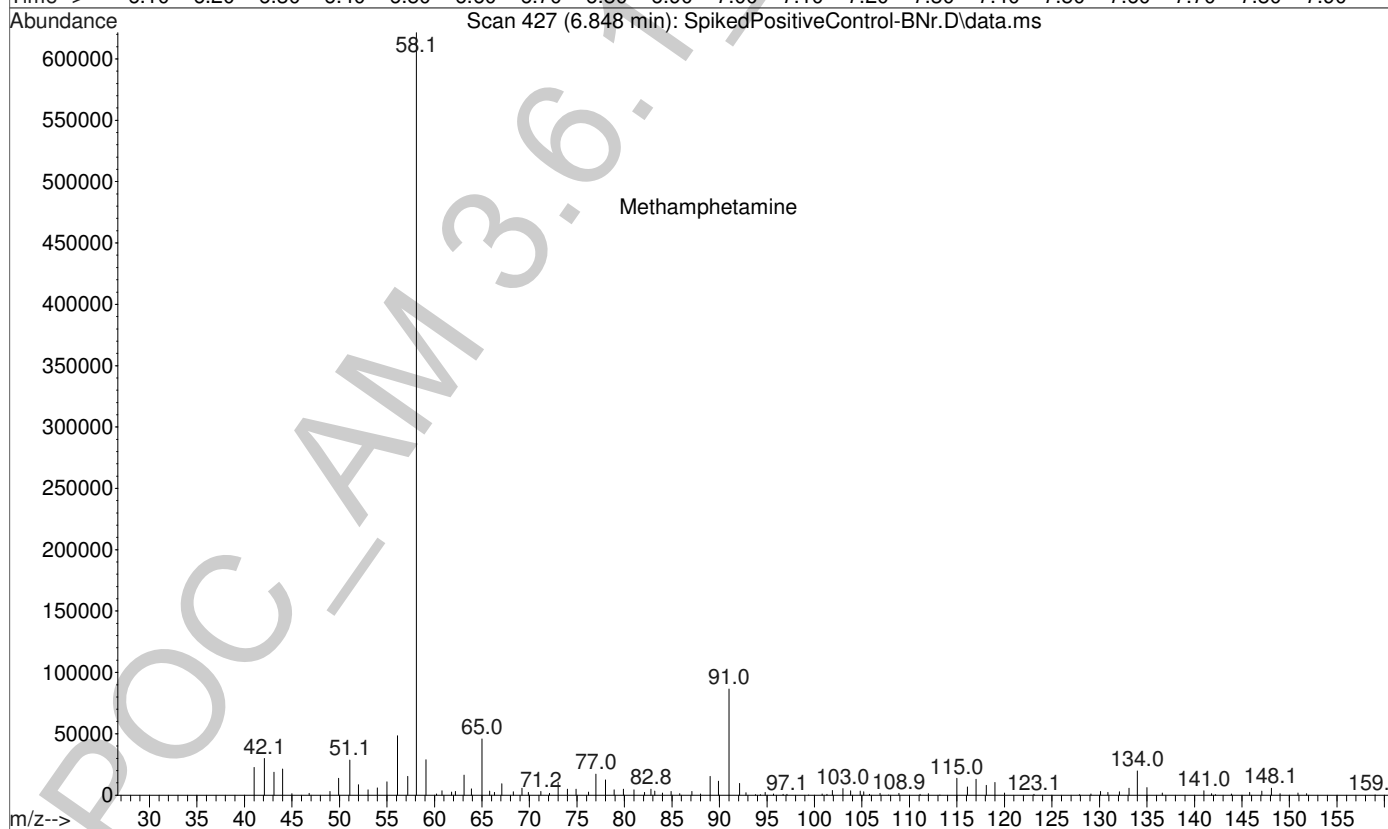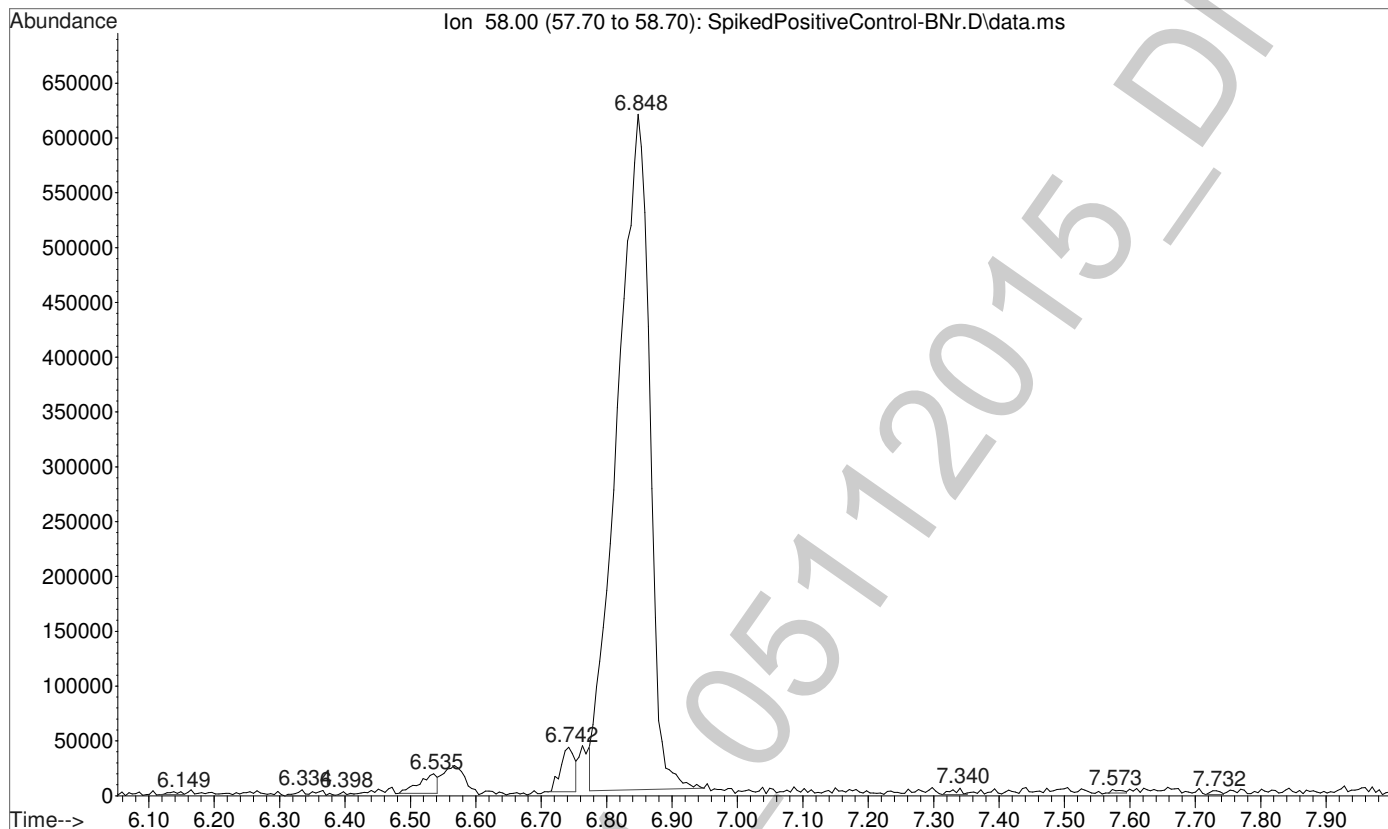



File :C:\gcms\1\data\Blood\051115BN\Reinjection Longer GC Method\S
... pikedPositiveControl-BNr.D
Operator : D Downey
Instrument : Probie
Acquired : 11 May 2015 19:30 using AcqMethod GBT092509.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

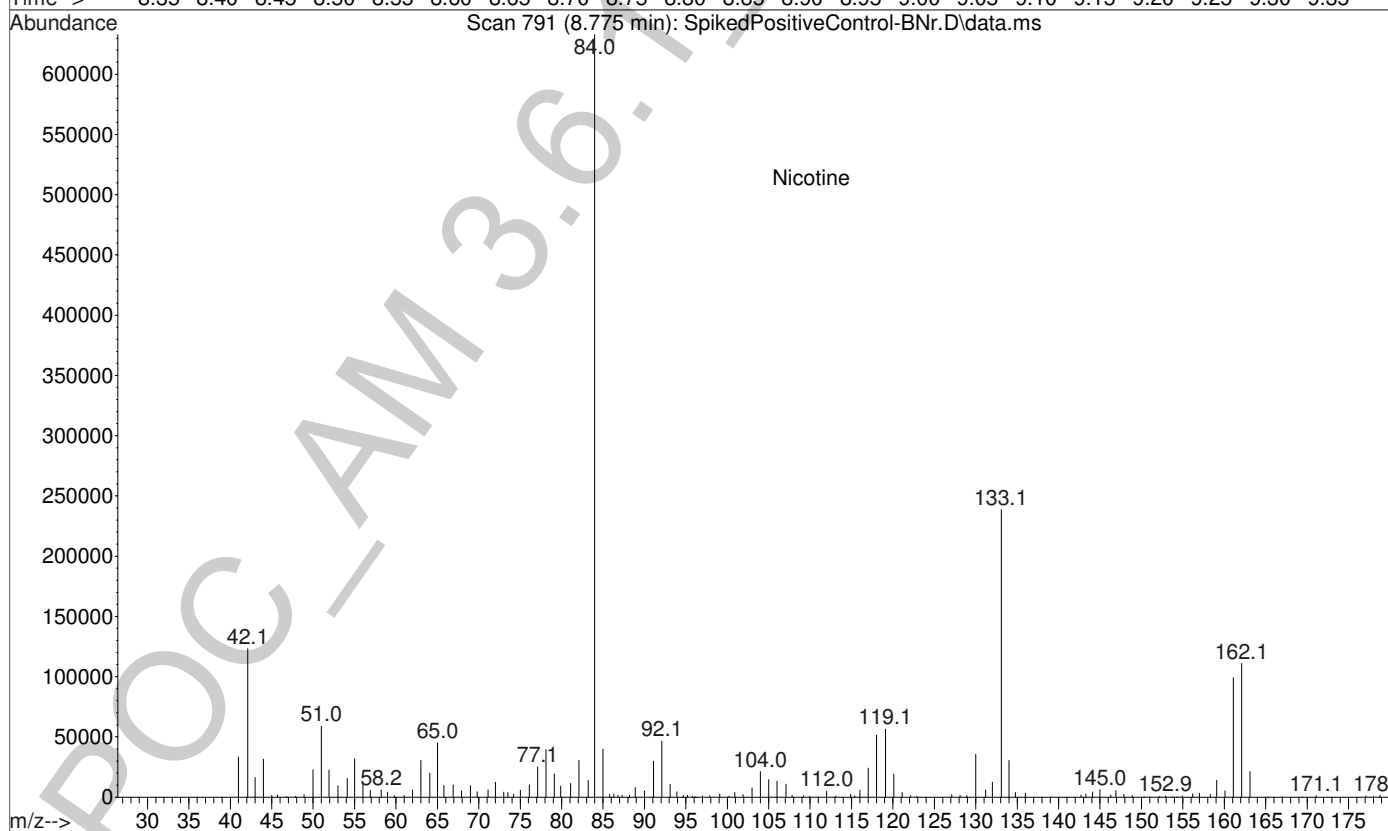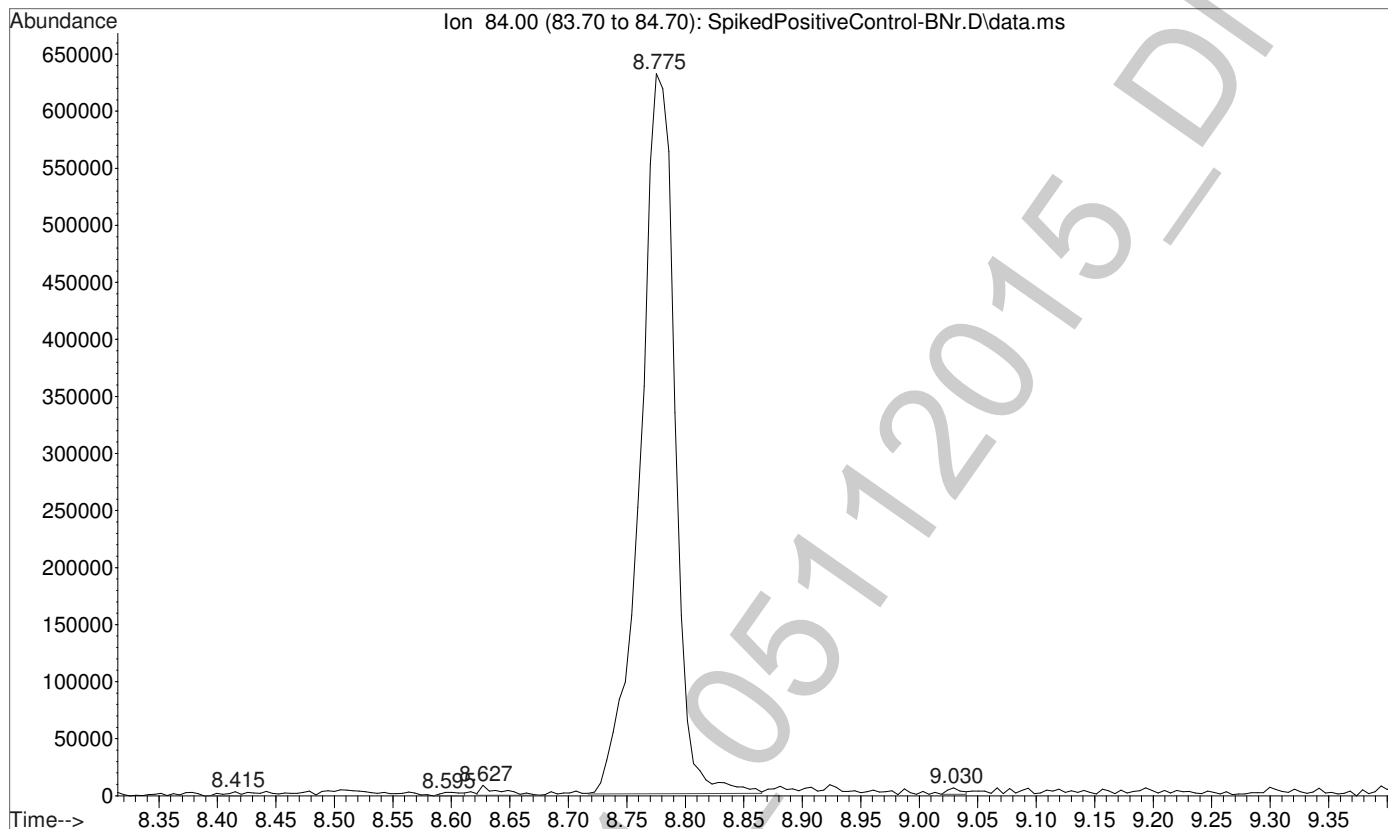



File :C:\gcms\1\data\Blood\051115BN\Reinjection Longer GC Method\S
... pikedPositiveControl-BNr.D
Operator : D Downey
Instrument : Probie
Acquired : 11 May 2015 19:30 using AcqMethod GBT092509.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

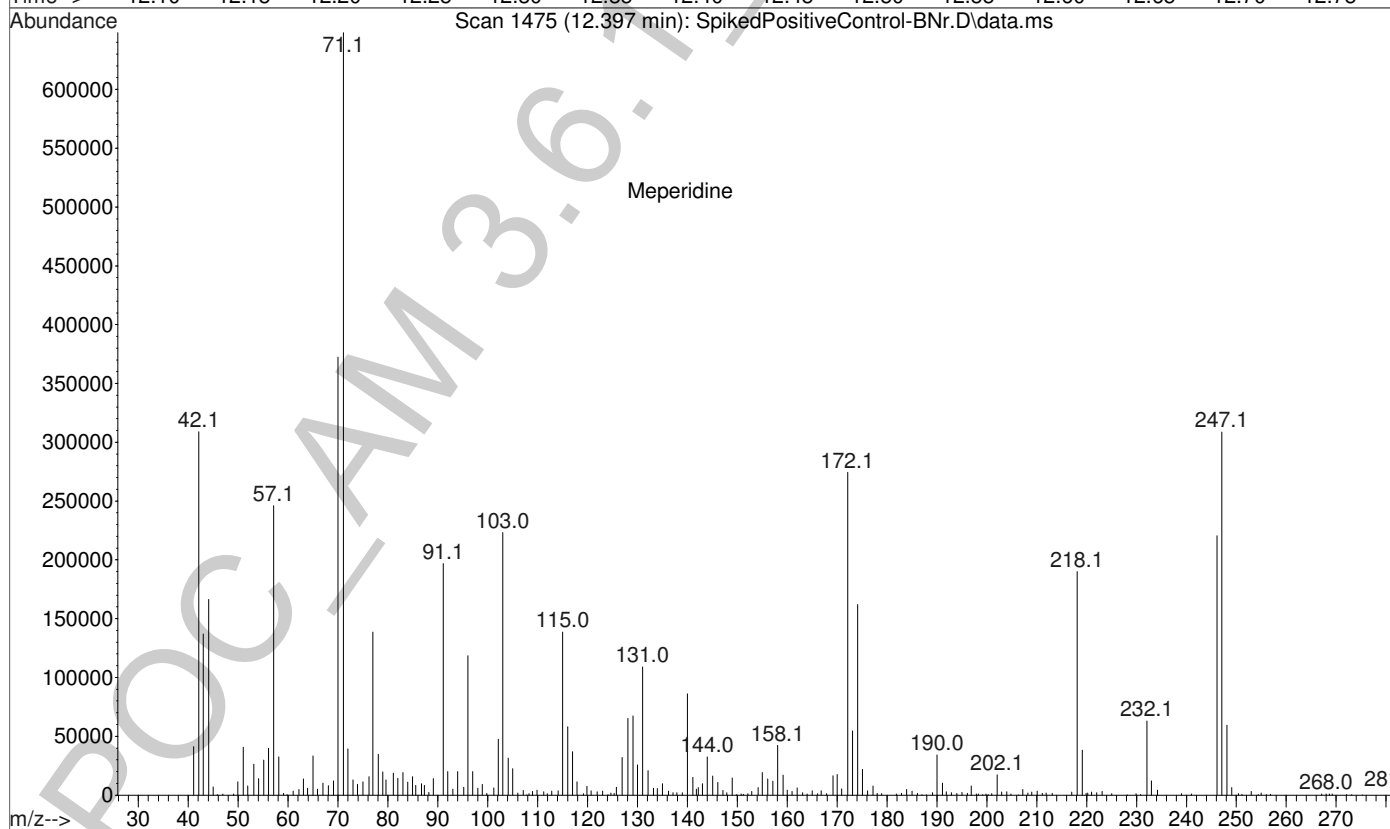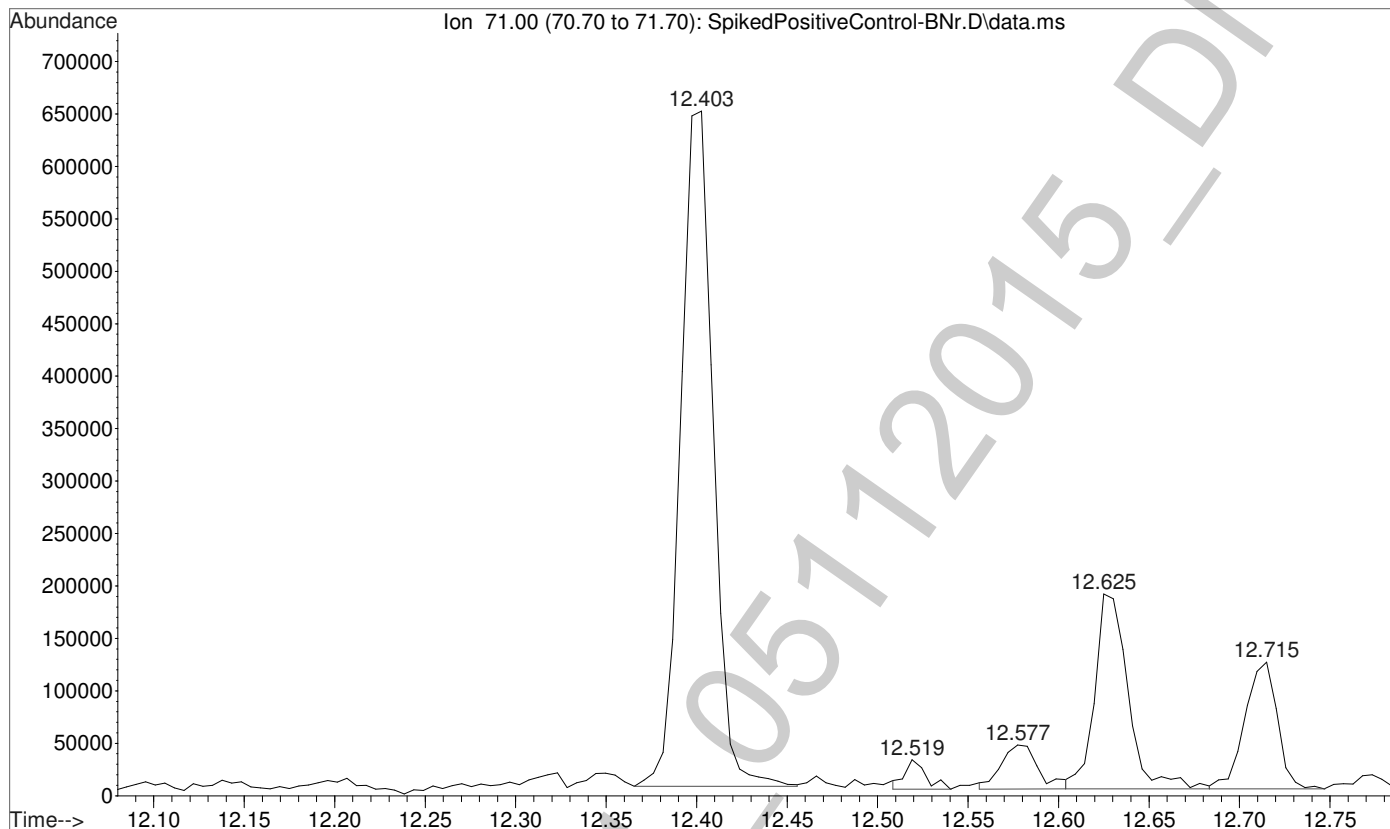



File :C:\gcms\1\data\Blood\051115BN\Reinjection Longer GC Method\S
... pikedPositiveControl-BNr.D
Operator : D Downey
Instrument : Probie
Acquired : 11 May 2015 19:30 using AcqMethod GBT092509.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

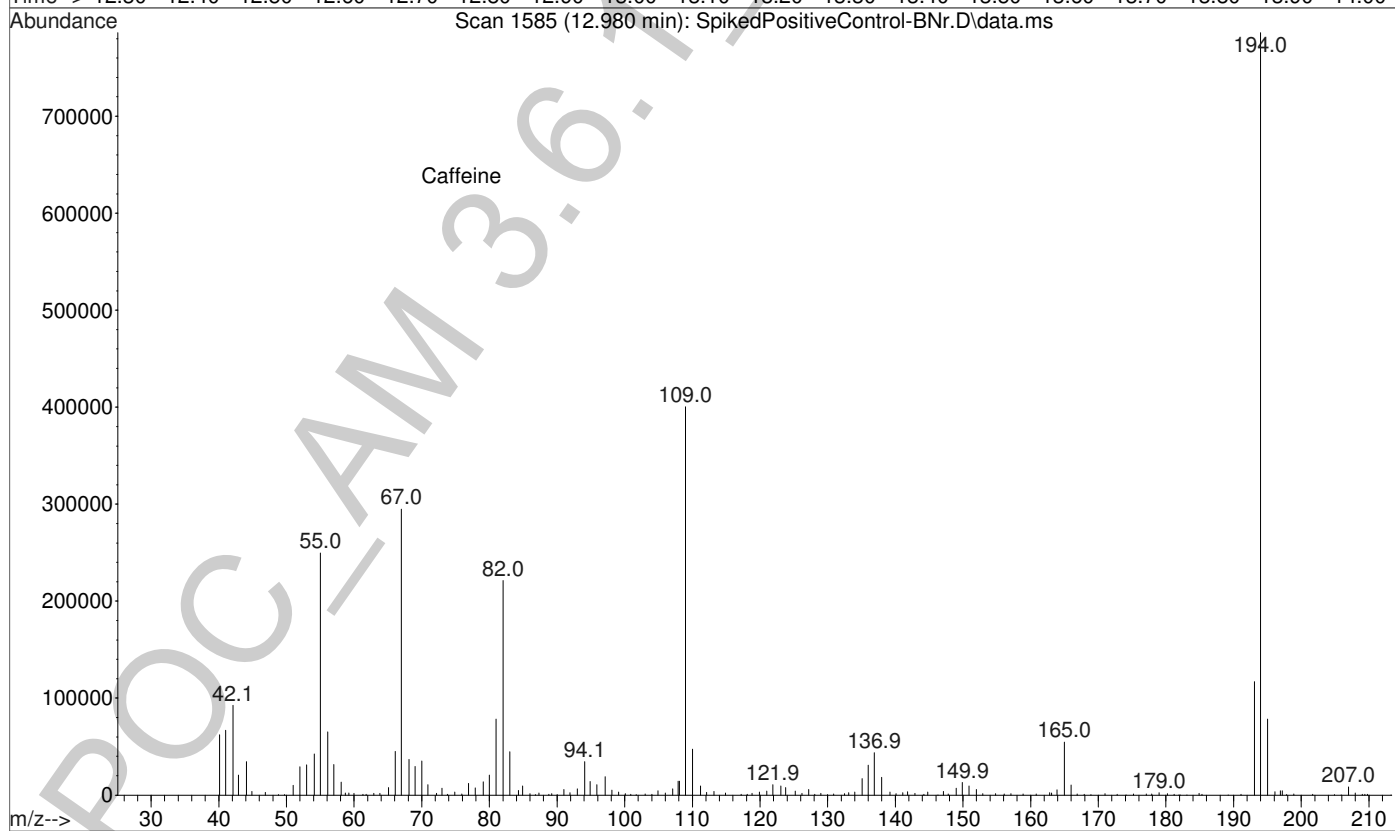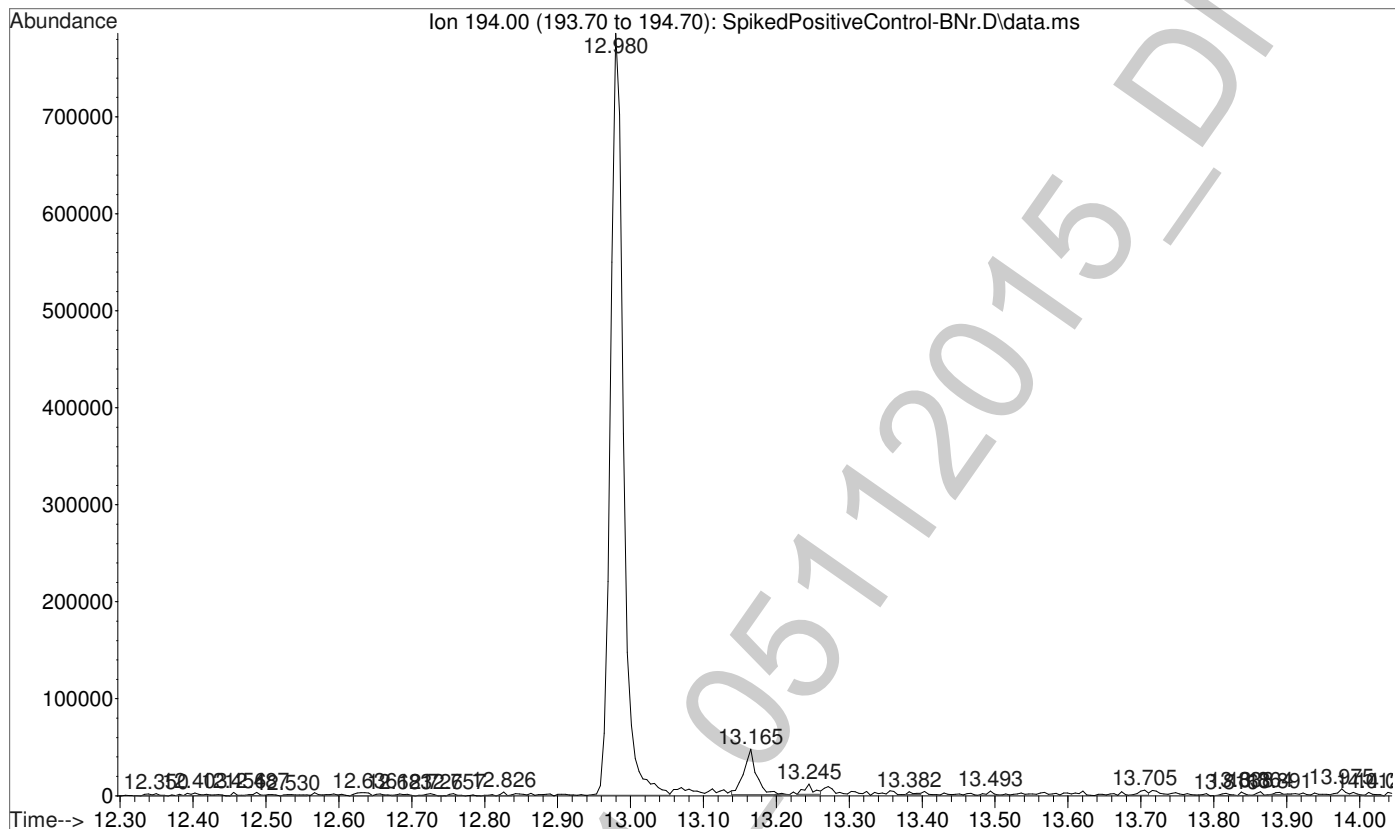



File :C:\gcms\1\data\Blood\051115BN\Reinjection Longer GC Method\S
... pikedPositiveControl-BNr.D
Operator : D Downey
Instrument : Probie
Acquired : 11 May 2015 19:30 using AcqMethod GBT092509.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

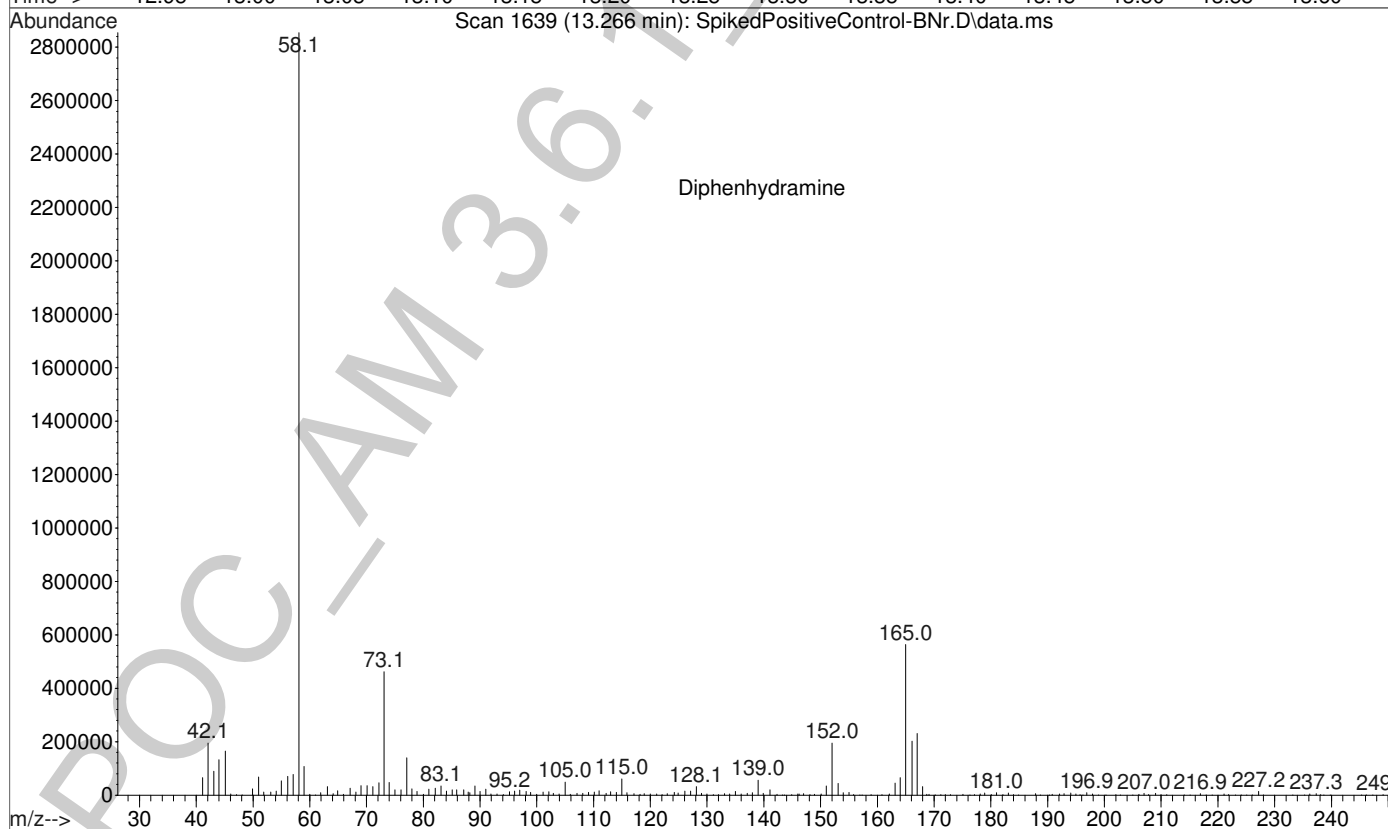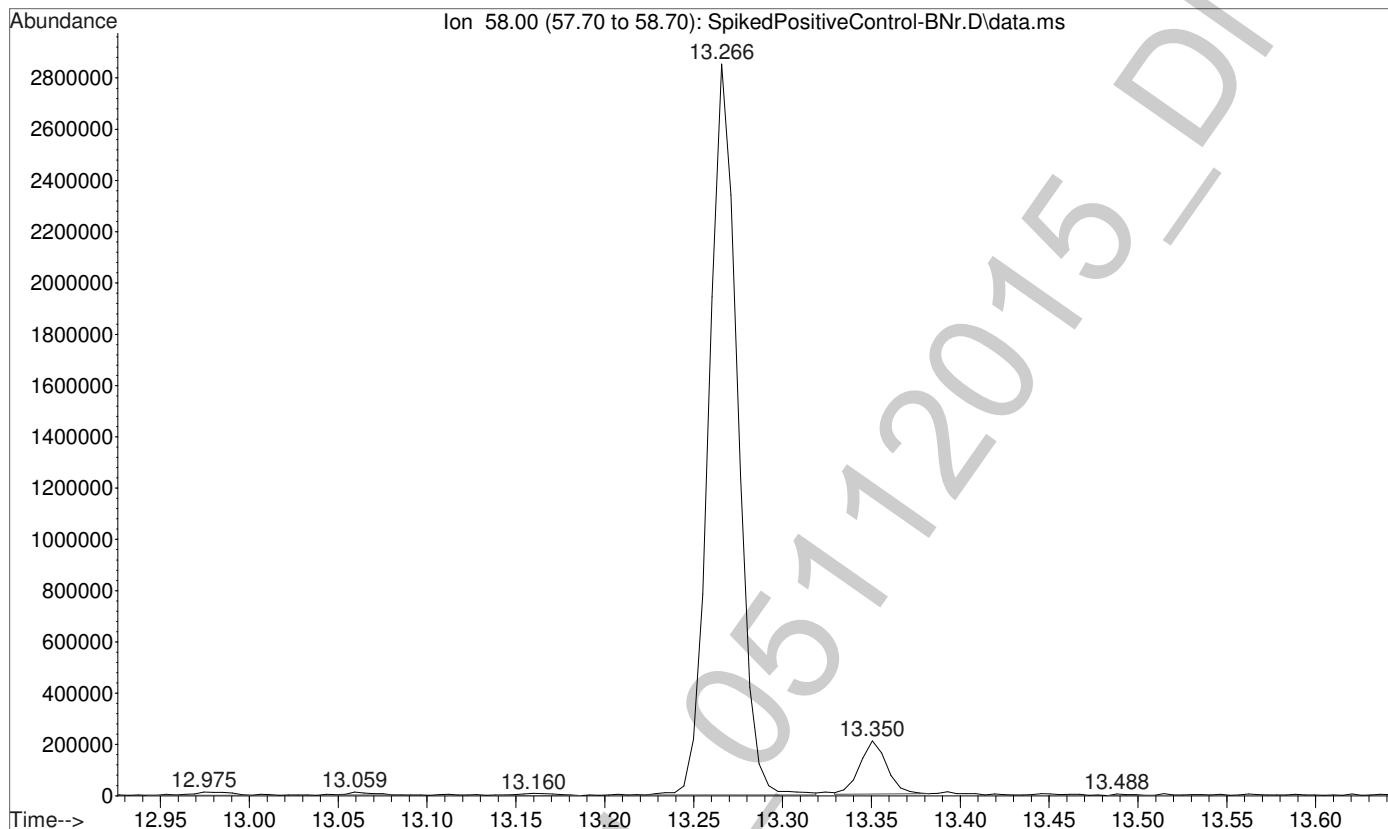



File :C:\gcms\1\data\Blood\051115BN\Reinjection Longer GC Method\S
... pikedPositiveControl-BNr.D
Operator : D Downey
Instrument : Probie
Acquired : 11 May 2015 19:30 using AcqMethod GBT092509.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

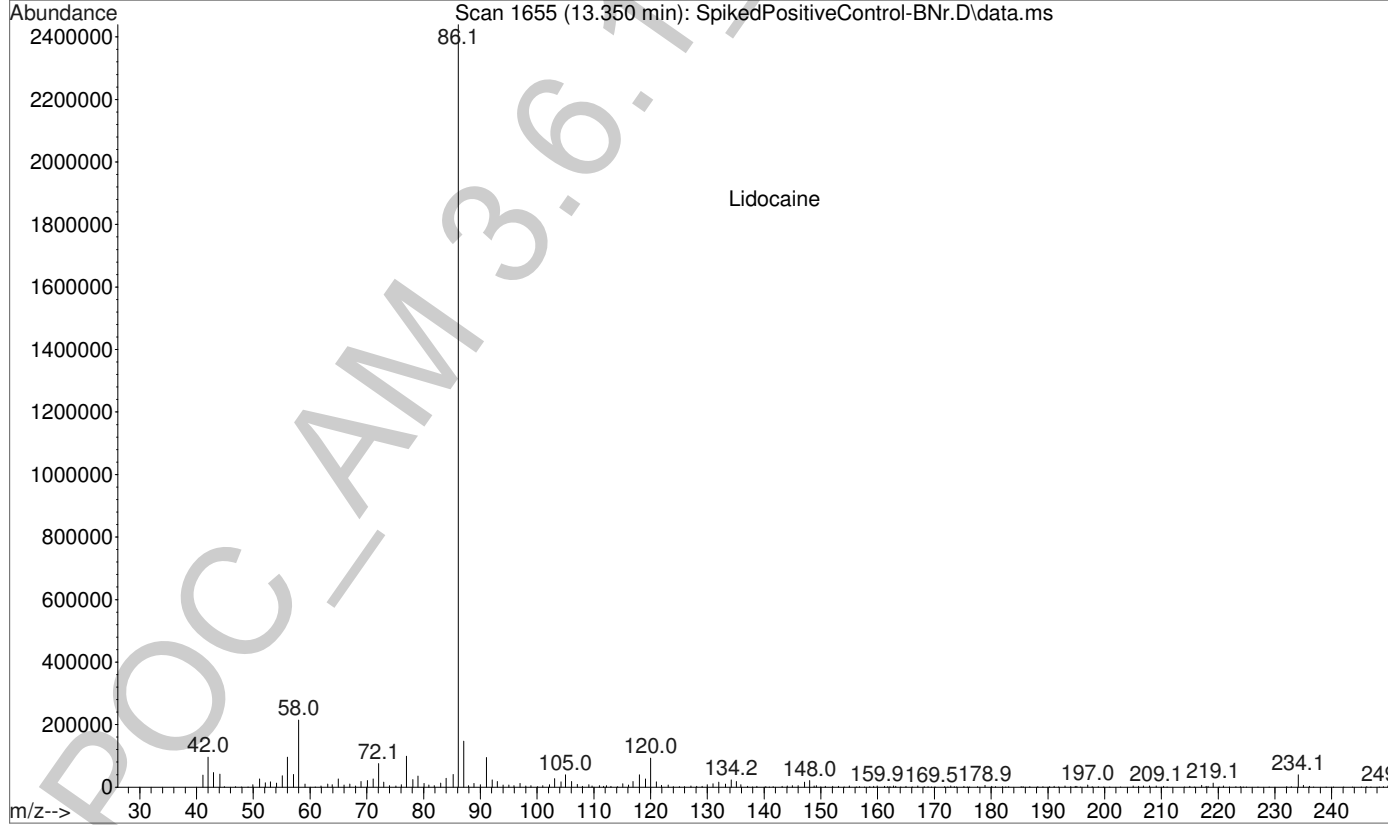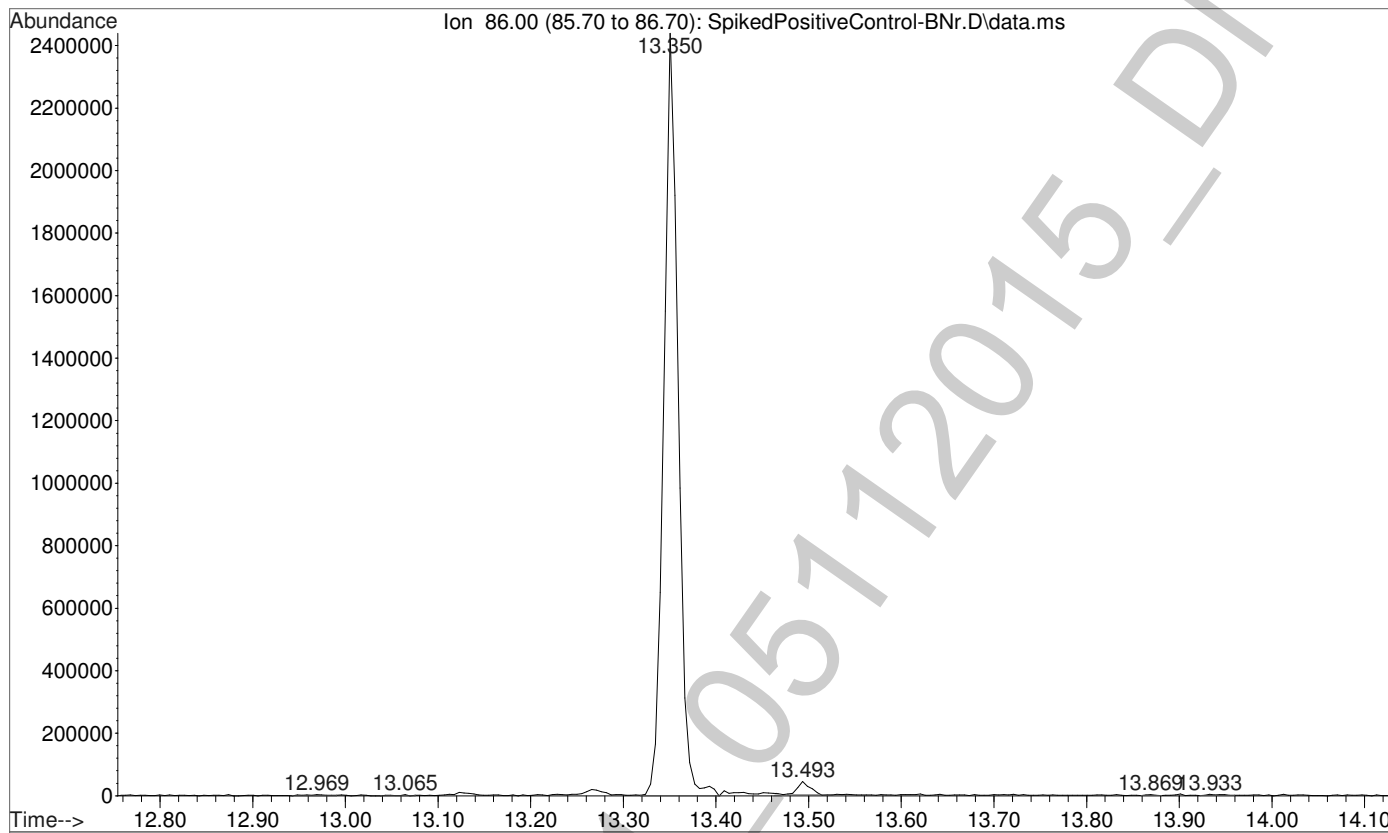



File :C:\gcms\1\data\Blood\051115BN\Reinjection Longer GC Method\S
... pikedPositiveControl-BNr.D
Operator : D Downey
Instrument : Probie
Acquired : 11 May 2015 19:30 using AcqMethod GBT092509.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

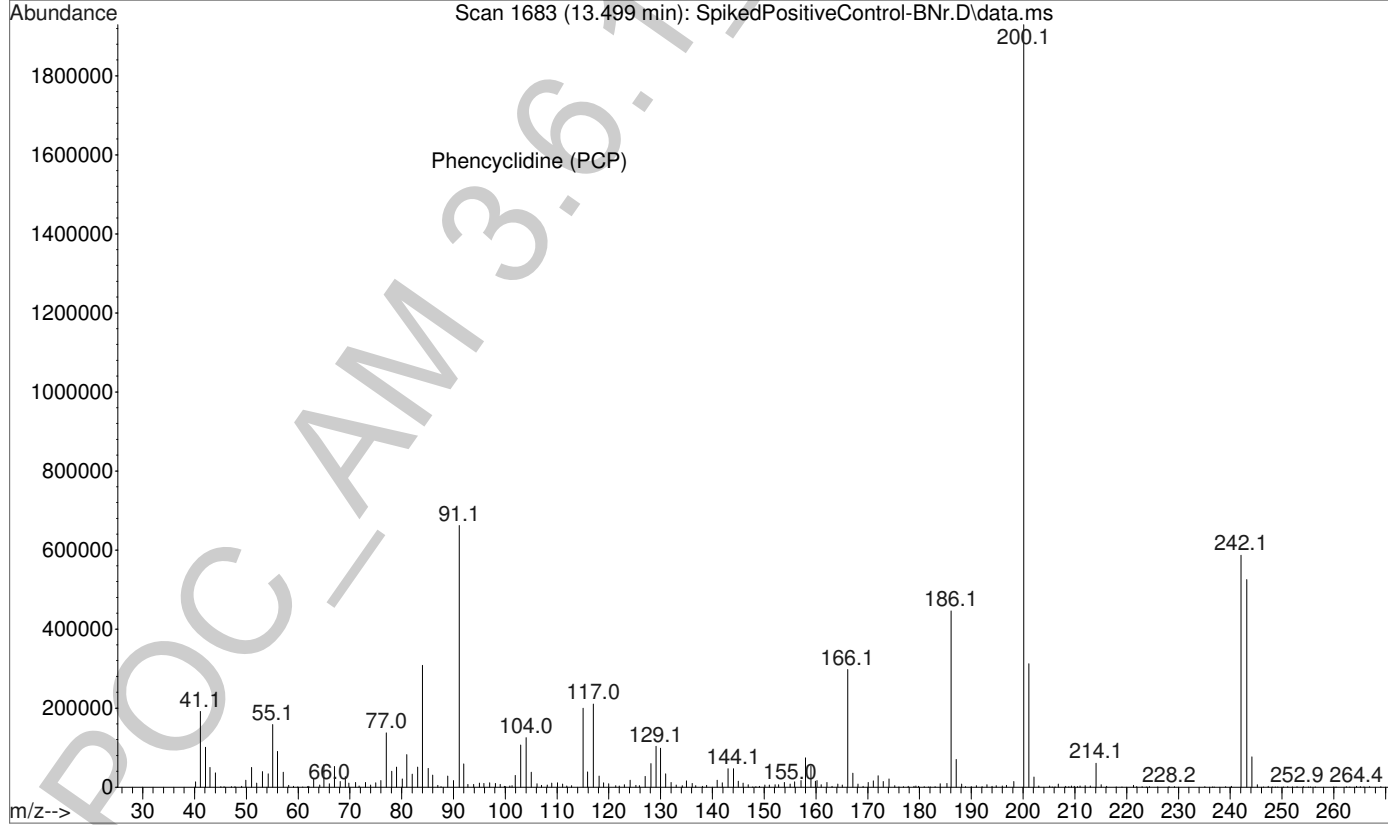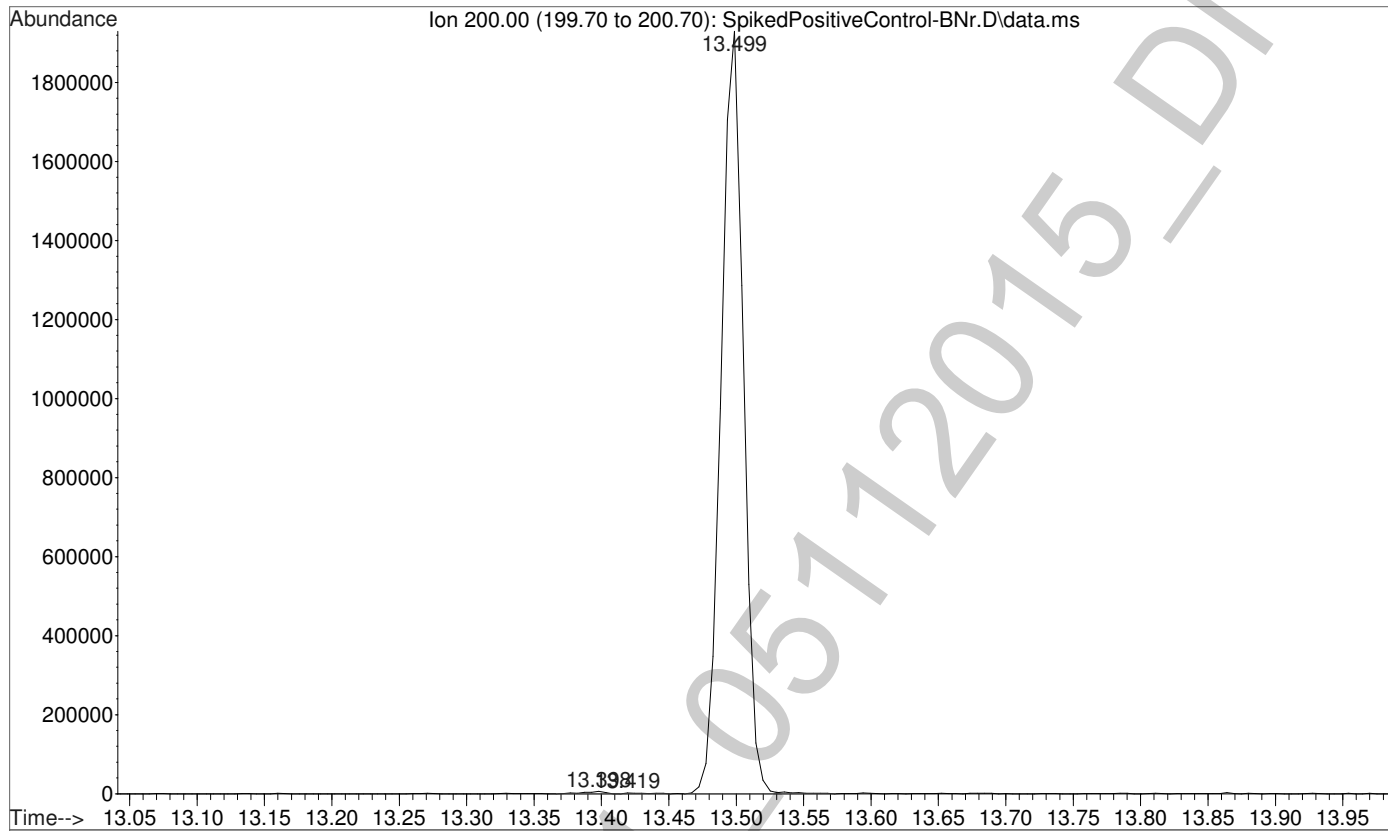



File :C:\gcms\1\data\Blood\051115BN\Reinjection Longer GC Method\S
... pikedPositiveControl-BNr.D
Operator : D Downey
Instrument : Probie
Acquired : 11 May 2015 19:30 using AcqMethod GBT092509.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

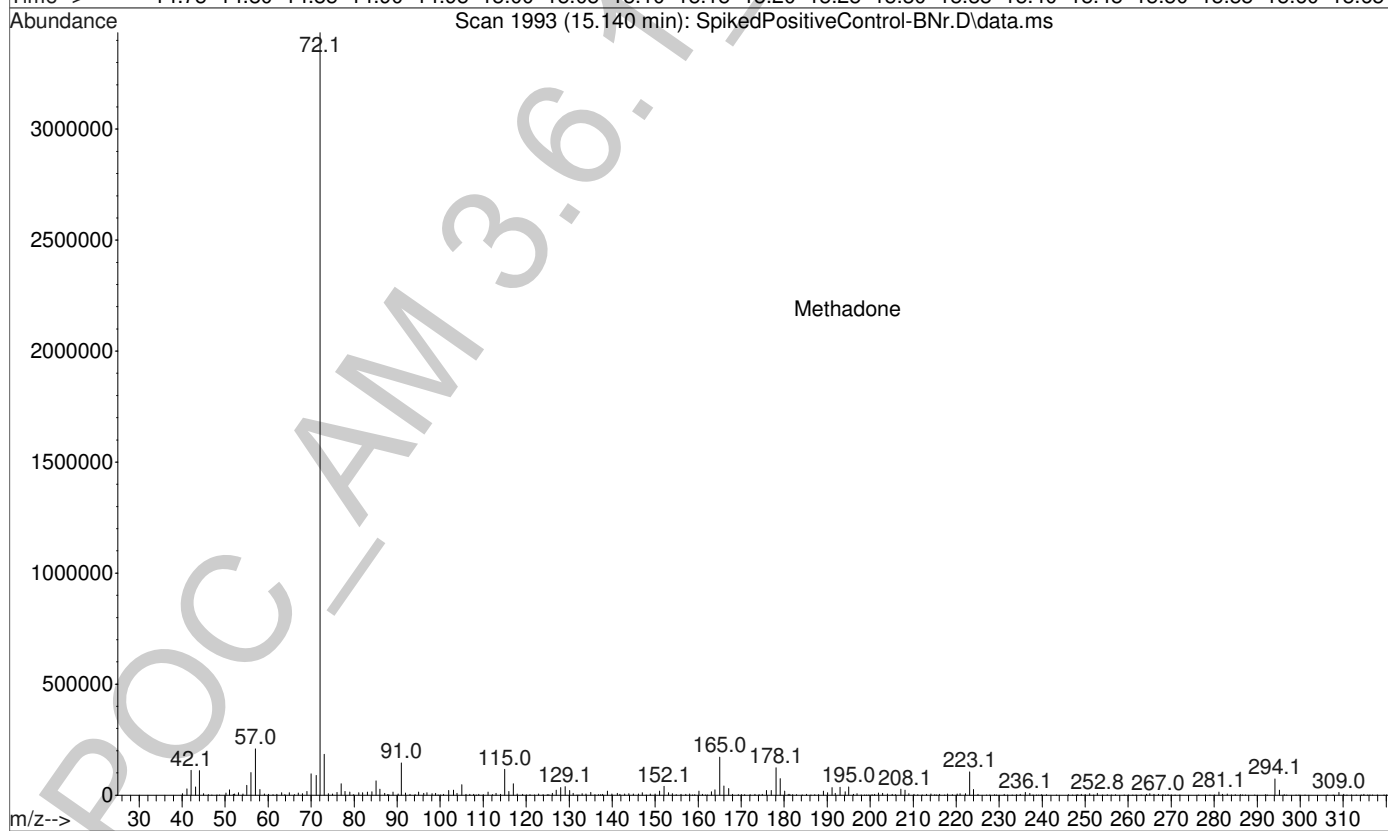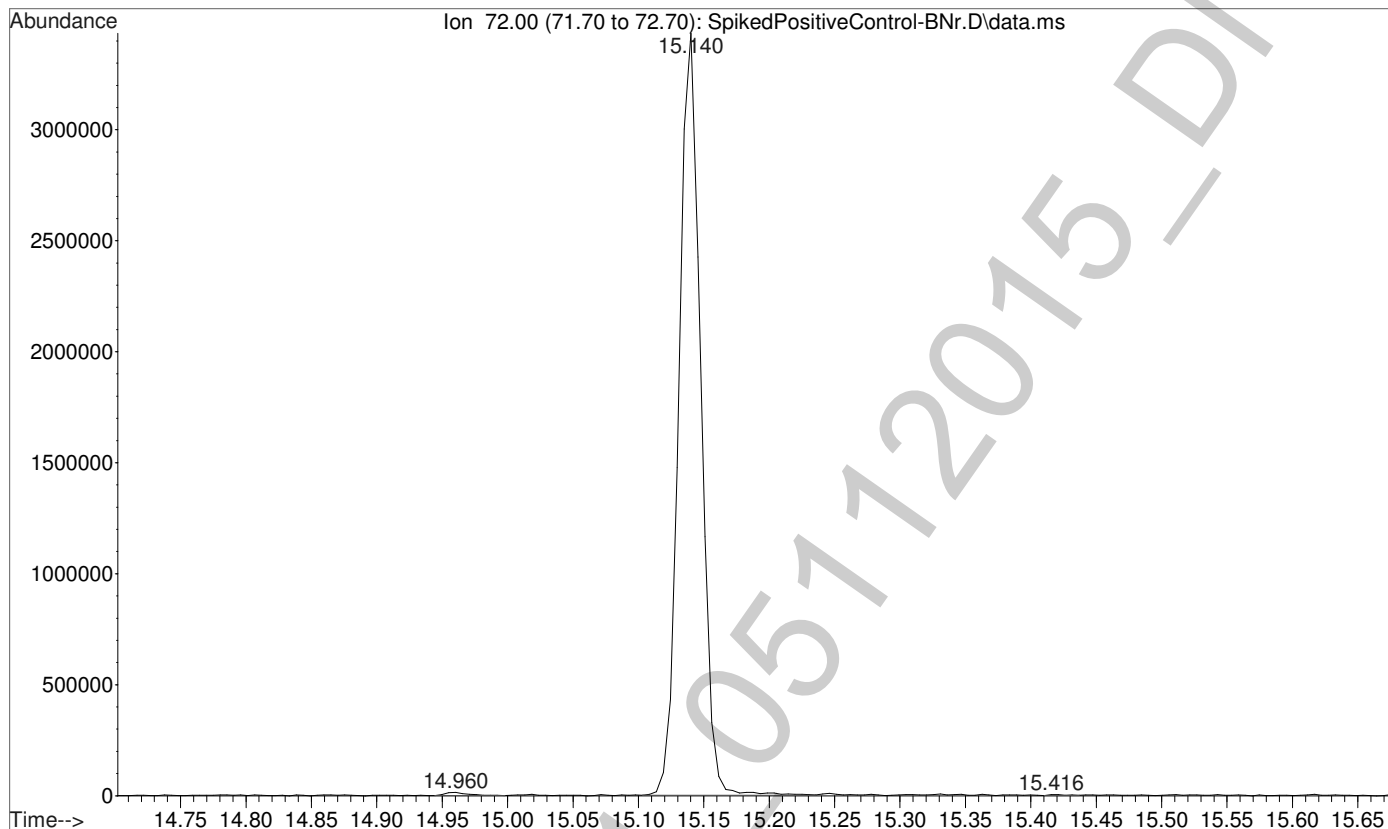



File :C:\gcms\1\data\Blood\051115BN\Reinjection Longer GC Method\S
... pikedPositiveControl-BNr.D
Operator : D Downey
Instrument : Probie
Acquired : 11 May 2015 19:30 using AcqMethod GBT092509.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

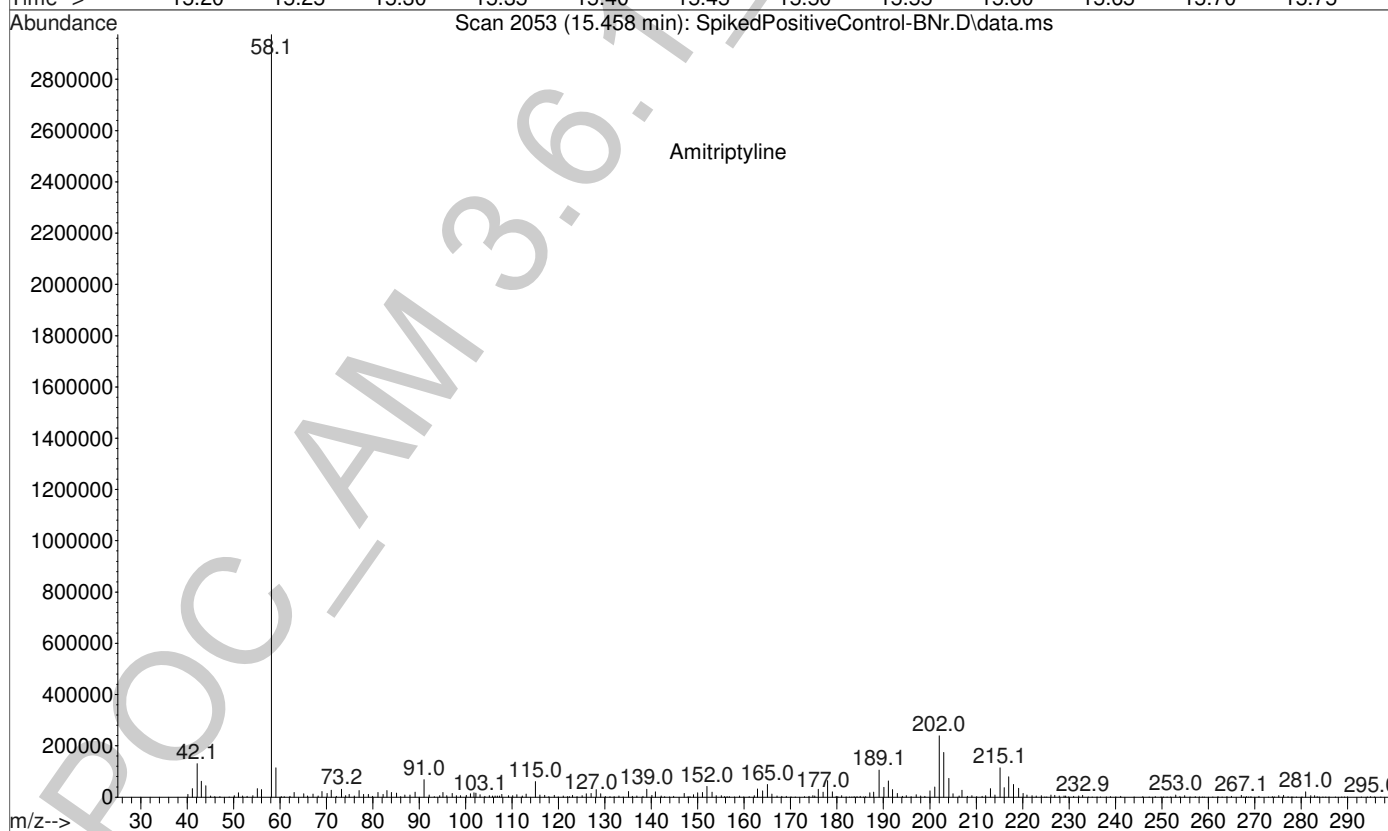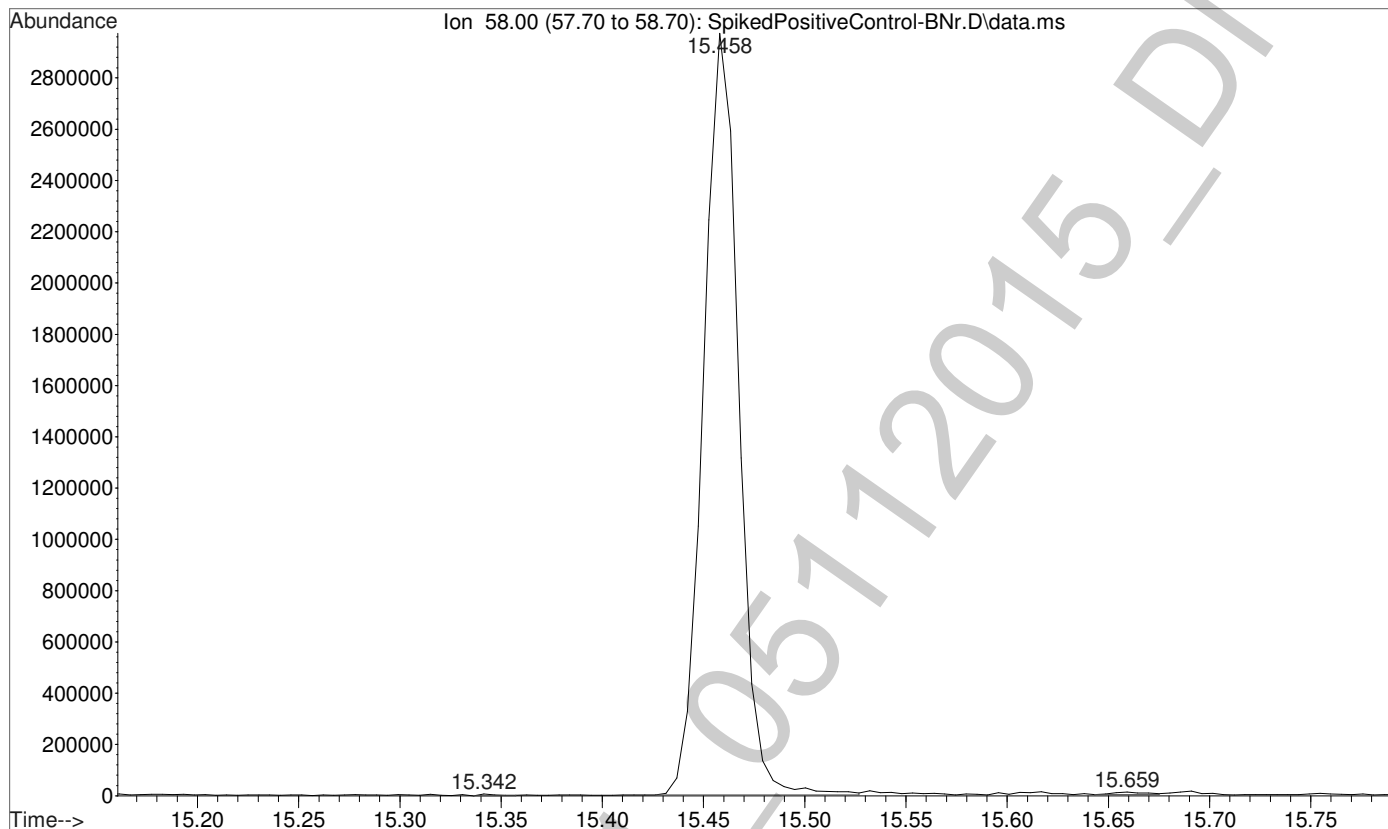



File :C:\gcms\1\data\Blood\051115BN\Reinjection Longer GC Method\S
... pikedPositiveControl-BNr.D
Operator : D Downey
Instrument : Probie
Acquired : 11 May 2015 19:30 using AcqMethod GBT092509.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

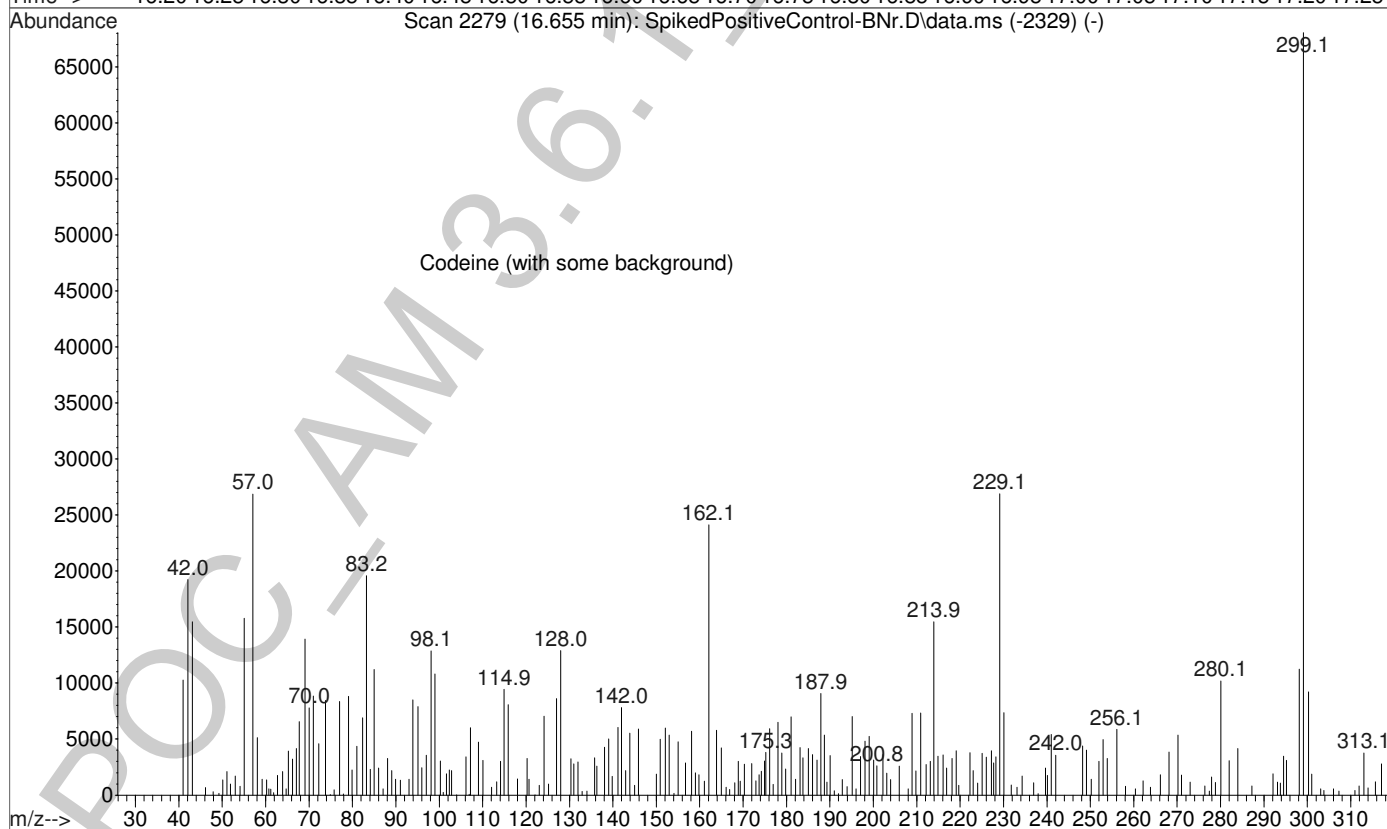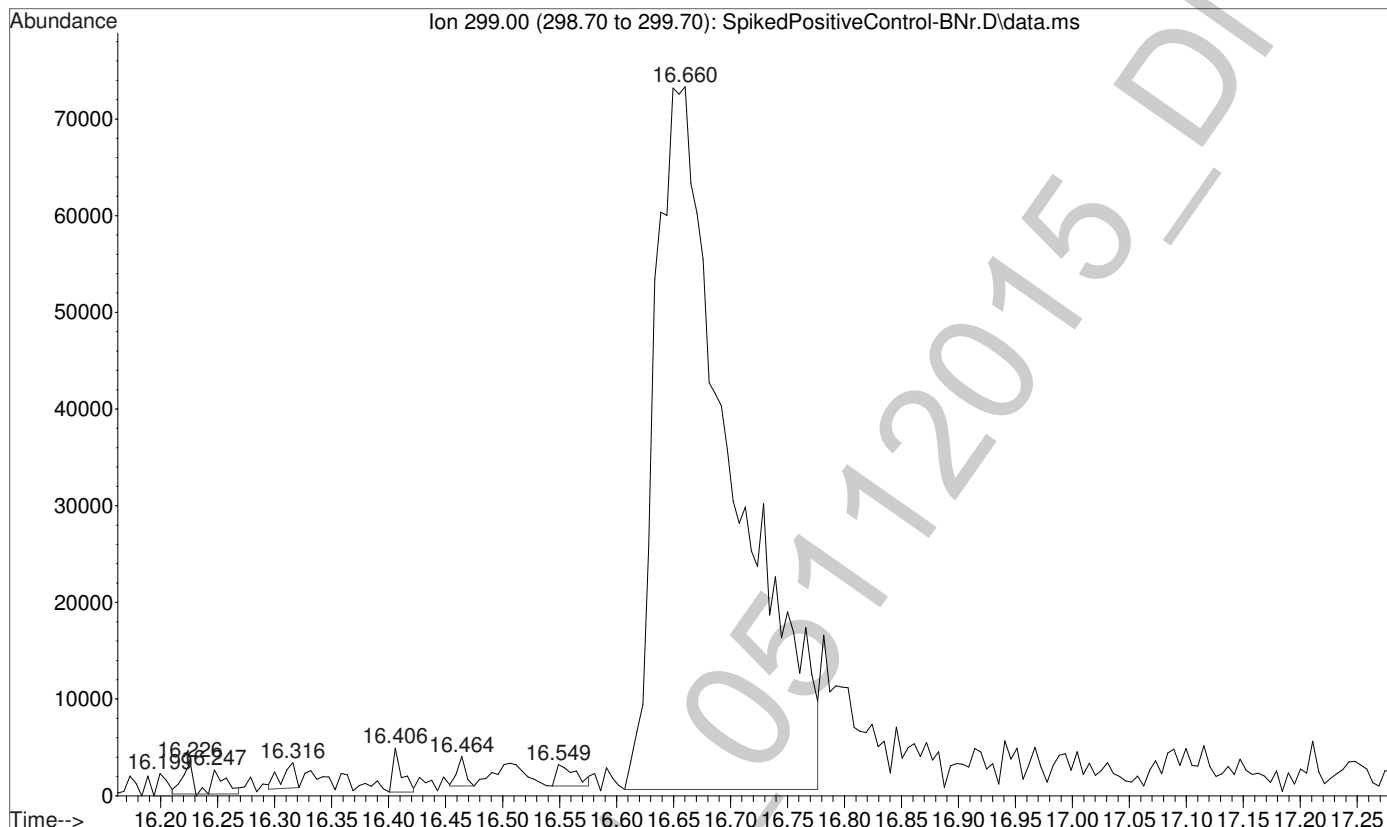



File :C:\gcms\1\data\Blood\051115BN\Reinjection Longer GC Method\S
... pikedPositiveControl-BNr.D
Operator : D Downey
Instrument : Probie
Acquired : 11 May 2015 19:30 using AcqMethod GBT092509.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

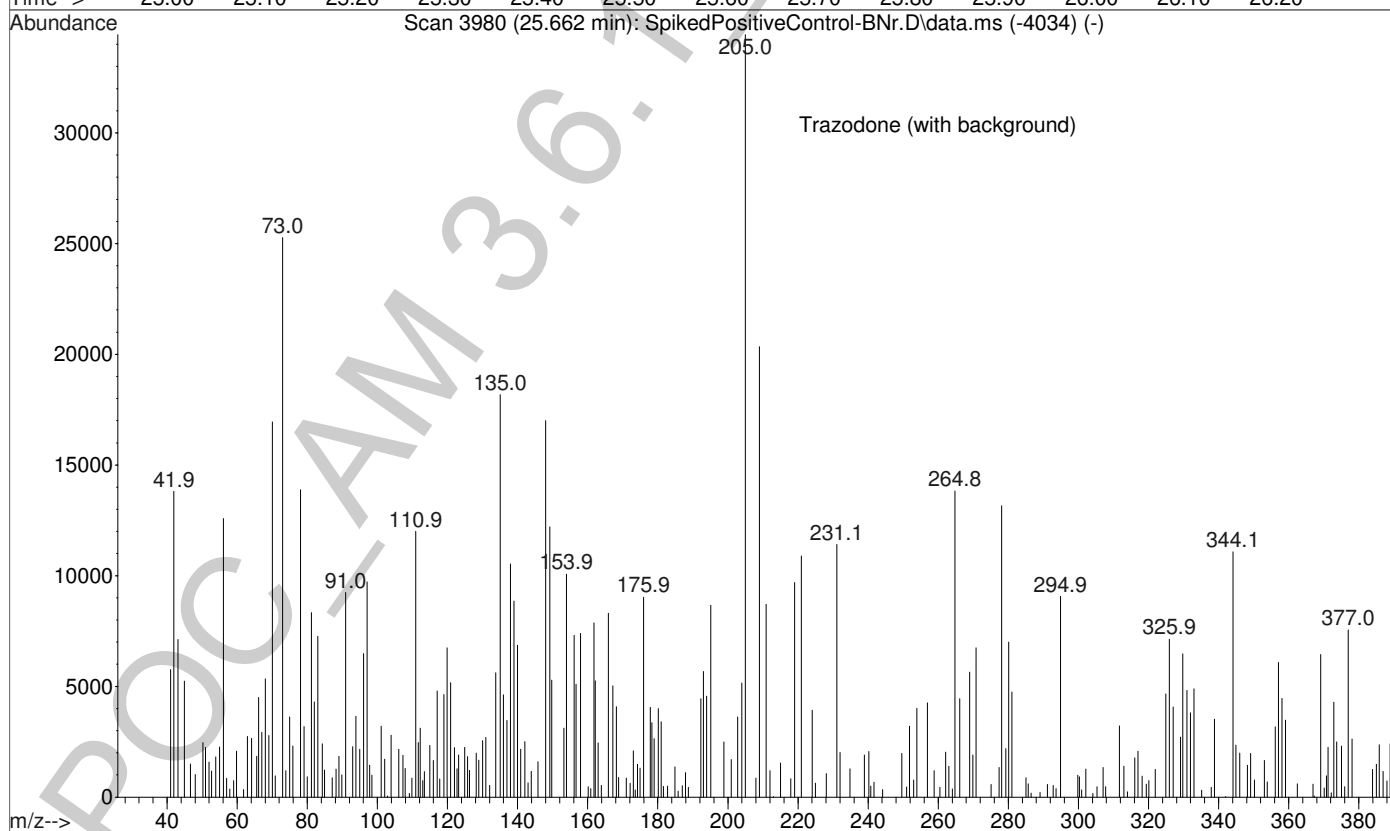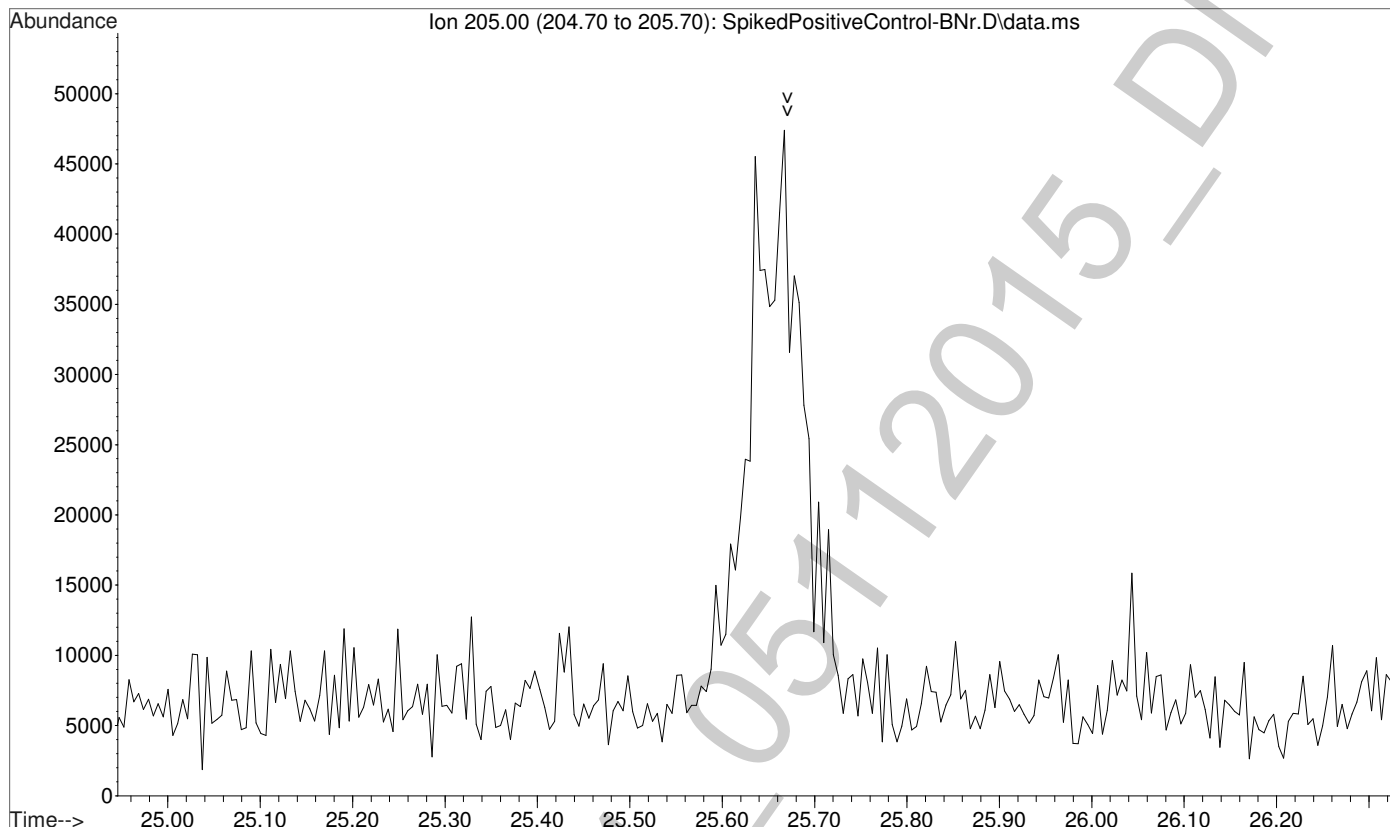

File :C:\gcms\1\data\Blood\051115BN\Reinjection Longer GC Method\p
... rbLK2r.D
Operator : D Downey
Instrument : Probie
Acquired : 11 May 2015 20:04 using AcqMethod GBT092509.M
Sample Name: Solvent Blank
Misc Info : Chloroform

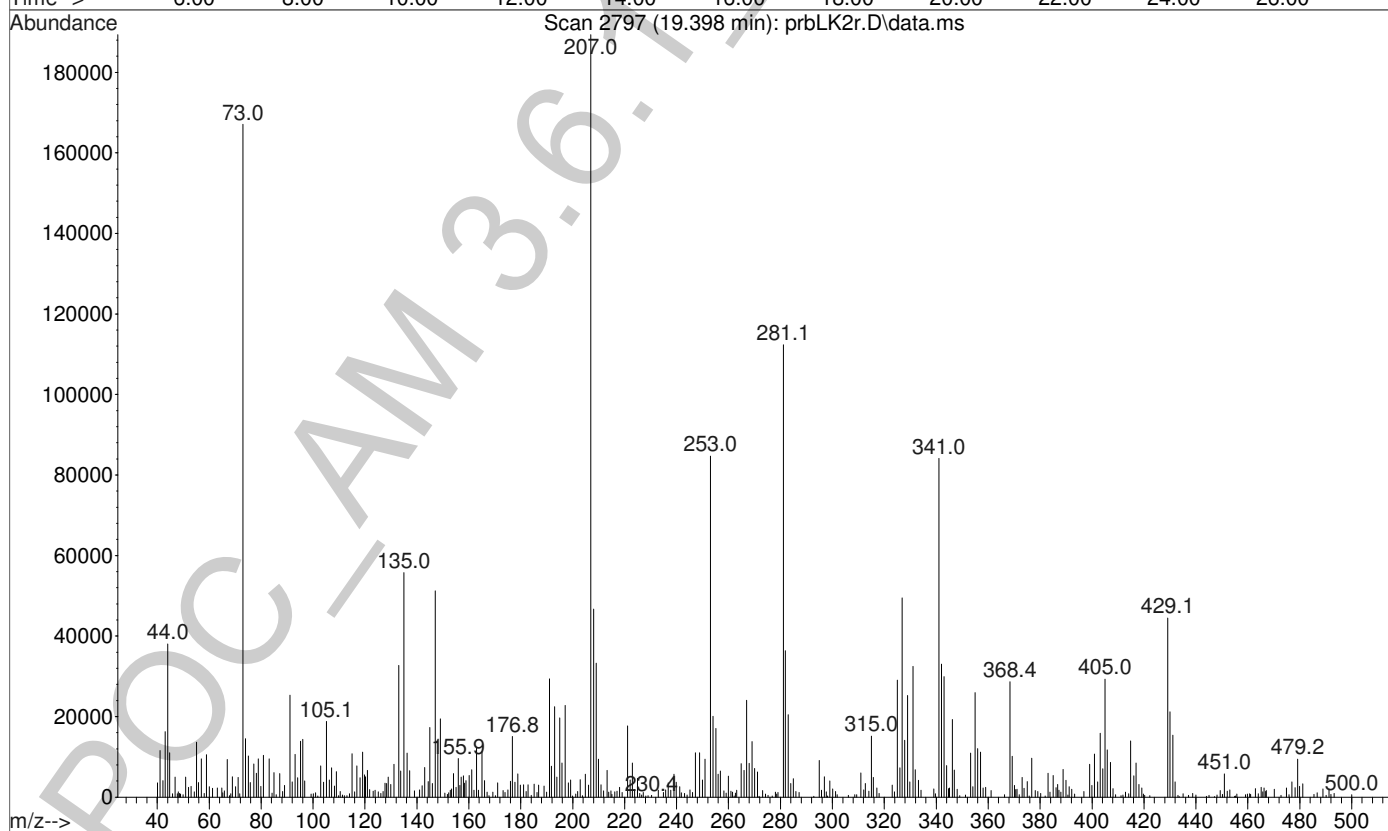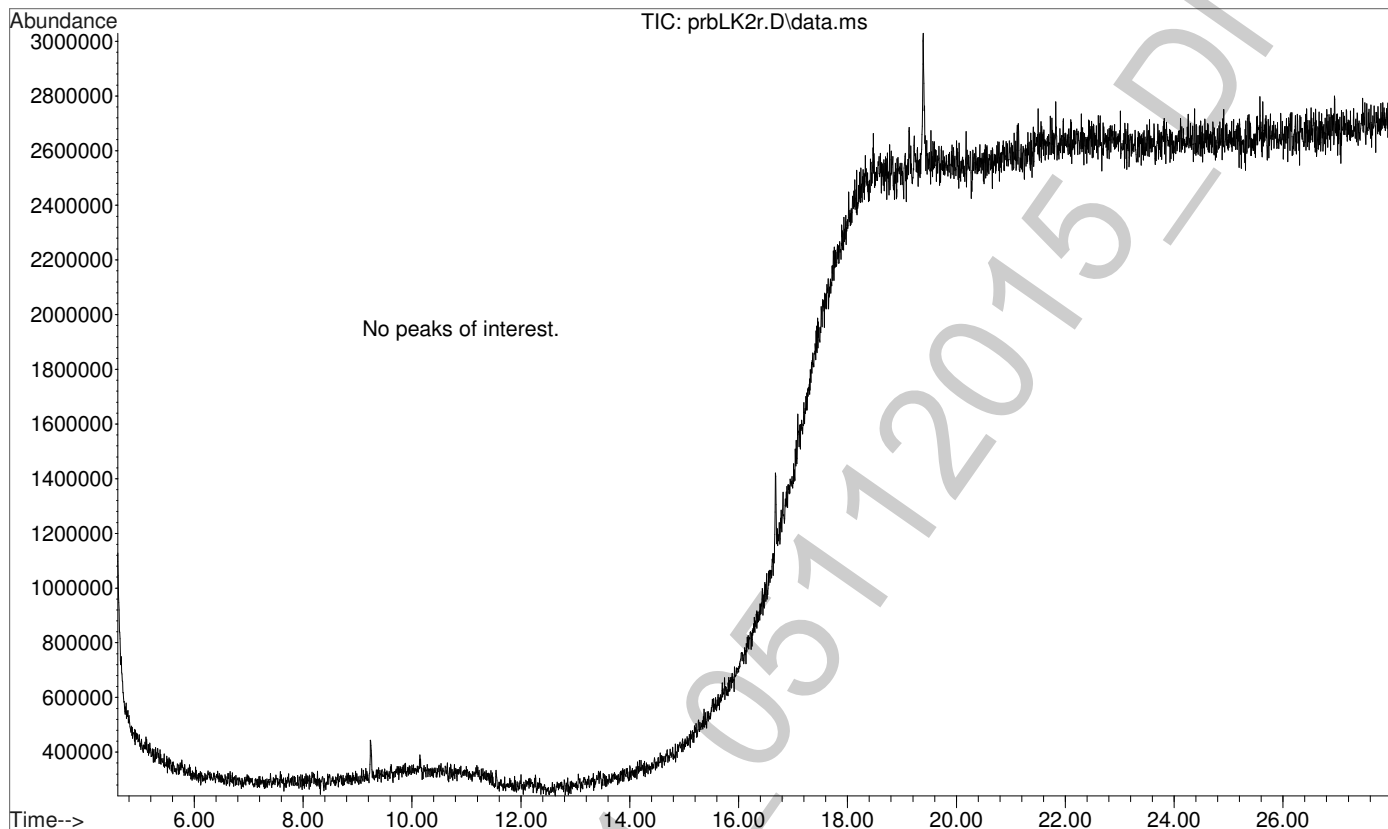

File :C:\gcms\1\data\Blood\051115BN\POSTBLKr.D
Operator : D Downey
Acquired : 11 May 2015 22:34 using AcqMethod GBT092509.M
Instrument : Probie
Sample Name: BLK
Misc Info : Chloroform
Vial Number: 97

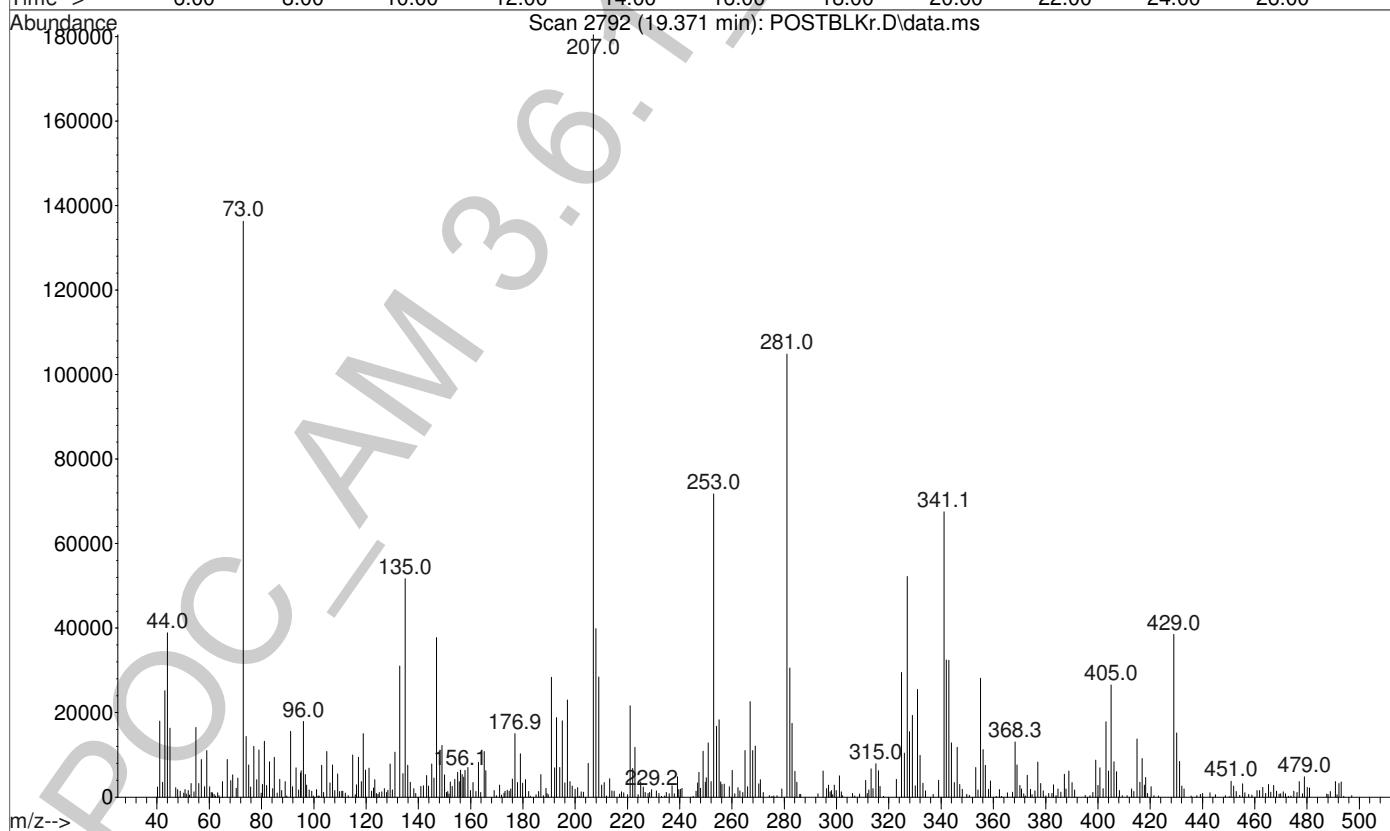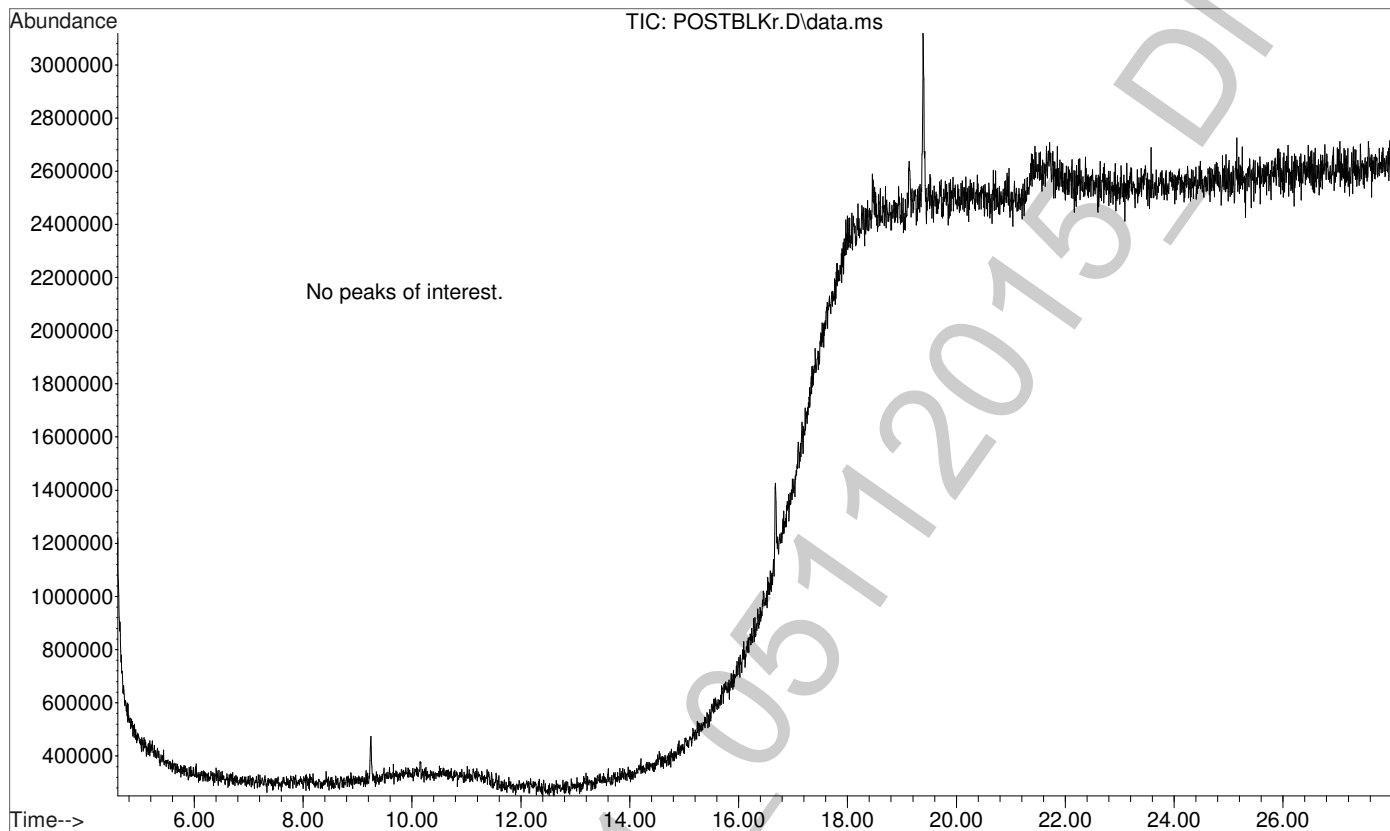

File :C:\gcms\1\data\Blood\051115BN\AFTER.D
Operator : D Downey
Acquired : 11 May 2015 23:09 using AcqMethod BNSB120510.M
Instrument : Probie
Sample Name: BLK
Misc Info : Chloroform
Vial Number: 96

