


How to download Performance Verification data using AlcoMark software




Attach the FC20 unit using a unit cable into a computer that contains the AlcoMark software.
Note: ISP agencies get the AlcoMark upgrade at no charge but a separate cable may have to be purchased from Lifeloc. This is the same cable used for the DataTrak software.



Double click the AlcoMark.exe icon to open the software

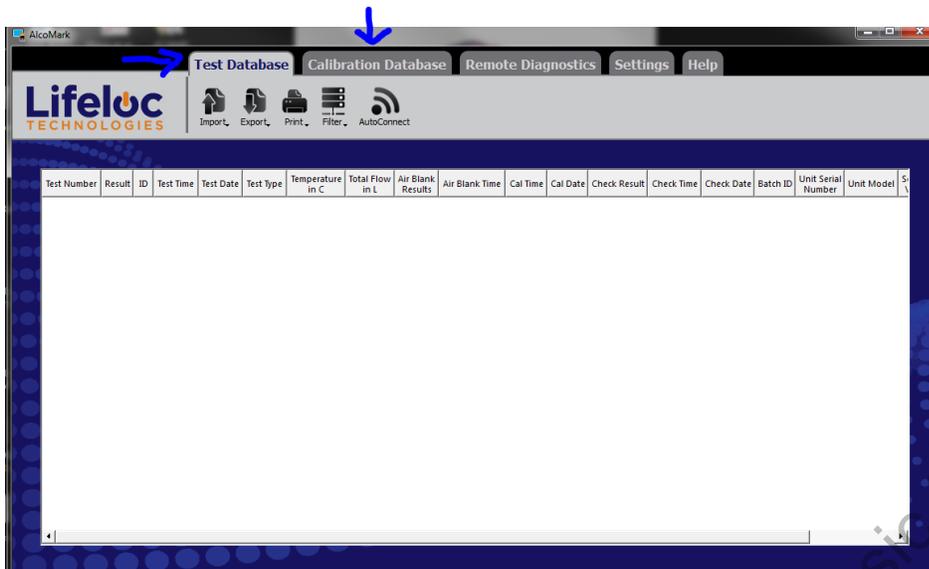

When the software first opens, take note to what tab is selected. The test database will view subject test results and the calibration database will view performance verification related records.

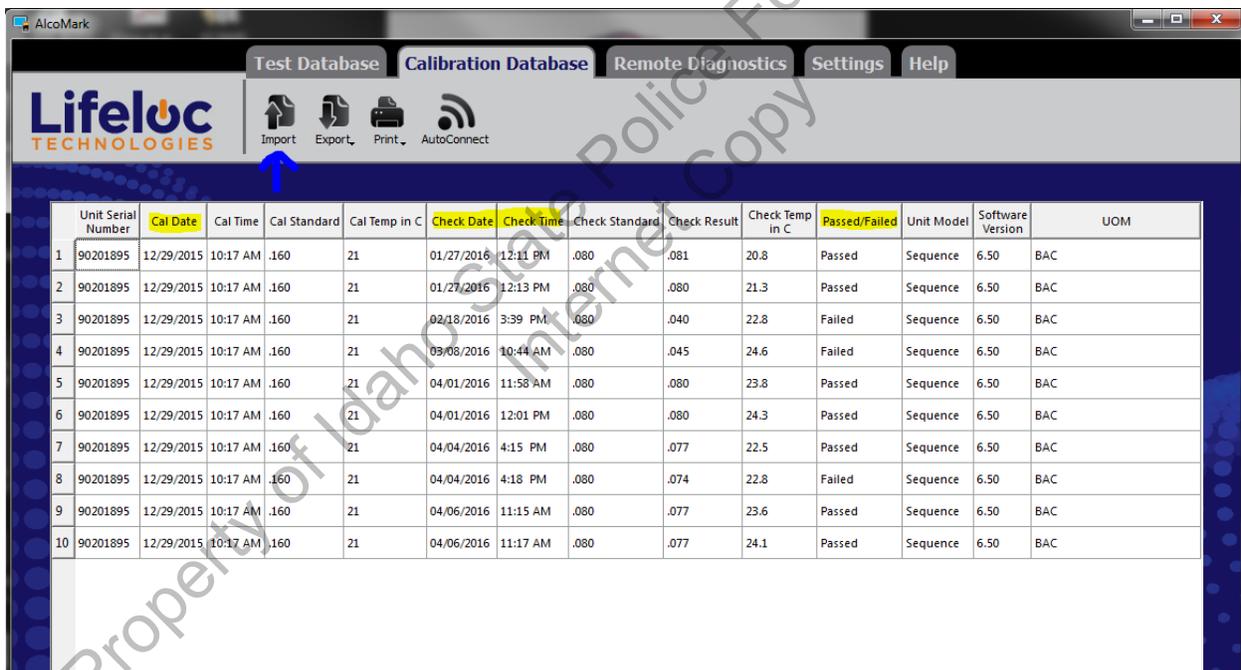

Click import. The data will be downloaded and can be viewed using this software. The Cal Date corresponds to when the instrument was last adjusted in the ISP Forensic Lab. Check date/time is when the PV was performed and other information. Note: the information viewed can be customized by going to settings and view.

AlcoMark

Test Database Calibration Database Remote Diagnostics Settings Help

Lifeloc TECHNOLOGIES

Import Export Print AutoConnect

	Unit Serial Number	Cal Date	Cal Time	Cal Standard	Cal Temp in C	Check Date	Check Time	Check Standard	Check Result	Check Temp in C	Passed/Failed	Unit Model	Software Version	UOM
1	90201895	12/29/2015	10:17 AM	.160	21	01/27/2016	12:11 PM	.080	.081	20.8	Passed	Sequence	6.50	BAC
2	90201895	12/29/2015	10:17 AM	.160	21	01/27/2016	12:13 PM	.080	.080	21.3	Passed	Sequence	6.50	BAC
3	90201895	12/29/2015	10:17 AM	.160	21	02/18/2016	3:39 PM	.080	.040	22.8	Failed	Sequence	6.50	BAC
4	90201895	12/29/2015	10:17 AM	.160	21	03/08/2016	10:44 AM	.080	.045	24.6	Failed	Sequence	6.50	BAC
5	90201895	12/29/2015	10:17 AM	.160	21	04/01/2016	11:58 AM	.080	.080	23.8	Passed	Sequence	6.50	BAC
6	90201895	12/29/2015	10:17 AM	.160	21	04/01/2016	12:01 PM	.080	.080	24.3	Passed	Sequence	6.50	BAC
7	90201895	12/29/2015	10:17 AM	.160	21	04/04/2016	4:15 PM	.080	.077	22.5	Passed	Sequence	6.50	BAC
8	90201895	12/29/2015	10:17 AM	.160	21	04/04/2016	4:18 PM	.080	.074	22.8	Failed	Sequence	6.50	BAC
9	90201895	12/29/2015	10:17 AM	.160	21	04/06/2016	11:15 AM	.080	.077	23.6	Passed	Sequence	6.50	BAC
10	90201895	12/29/2015	10:17 AM	.160	21	04/06/2016	11:17 AM	.080	.077	24.1	Passed	Sequence	6.50	BAC

Highlight the data that needs to be printed out. (Note: right click the mouse on the row number to delete data. This will delete the data in AlcoMark but can always be re-imported from the unit).

AlcoMark

Test Database Calibration Database Remote Diagnostics Settings Help

Lifeloc TECHNOLOGIES

Print Preview: document1

66.3%

1 / 1

Unit Serial Number	Cal Date	Cal Time	Cal Standard	Cal Temp in C	Check Date	Check Time	Check Standard	Check Result	Check Temp in C	Passed/Failed	Unit Model	Software Version	UOM	
1	90201895	12/29/2015	10:17 AM	.160	21	01/27/2016	12:11 PM	.080	.081	20.8	Passed	Sequence	6.50	BAC
2	90201895	12/29/2015	10:17 AM	.160	21	01/27/2016	12:13 PM	.080	.080	21.3	Passed	Sequence	6.50	BAC
3	90201895	12/29/2015	10:17 AM	.160	21	02/18/2016	3:39 PM	.080	.040	22.8	Failed	Sequence	6.50	BAC
4	90201895	12/29/2015	10:17 AM	.160	21	03/08/2016	10:44 AM	.080	.045	24.6	Failed	Sequence	6.50	BAC
5	90201895	12/29/2015	10:17 AM	.160	21	04/01/2016	11:58 AM	.080	.080	23.8	Passed	Sequence	6.50	BAC
6	90201895	12/29/2015	10:17 AM	.160	21	04/01/2016	12:01 PM	.080	.080	24.3	Passed	Sequence	6.50	BAC
7	90201895	12/29/2015	10:17 AM	.160	21	04/04/2016	4:15 PM	.080	.077	22.5	Passed	Sequence	6.50	BAC
8	90201895	12/29/2015	10:17 AM	.160	21	04/04/2016	4:18 PM	.080	.074	22.8	Failed	Sequence	6.50	BAC
9	90201895	12/29/2015	10:17 AM	.160	21	04/06/2016	11:15 AM	.080	.077	23.6	Passed	Sequence	6.50	BAC
10	90201895	12/29/2015	10:17 AM	.160	21	04/06/2016	11:17 AM	.080	.077	24.1	Passed	Sequence	6.50	BAC

Print Preview: document1

Lifeloc Technologies Calibration / Check Printout

Sequence	6.50
Serial No	90201895
UOM	BAC
Last Check	04/04/2016
Time	4:18 PM
Cal Standard	.080
Result	074
Last Cal	12/29/2015
Time	10:17 AM
Cal Standard	.160

Lifeloc Technologies Calibration / Check Printout

Sequence	6.50
Serial No	90201895
UOM	BAC
Last Check	04/06/2016
Time	11:15 AM
Cal Standard	.080
Result	077
Last Cal	12/29/2015
Time	10:17 AM
Cal Standard	.160

Lifeloc Technologies Calibration / Check Printout

Sequence	6.50
Serial No	90201895
UOM	BAC
Last Check	04/06/2016
Time	11:17 AM
Cal Standard	.080
Result	077
Last Cal	12/29/2015
Time	10:17 AM
Cal Standard	.160

Print or save the pdf file.

The screenshot displays the AlcoMark software interface with a Microsoft Excel spreadsheet open. The spreadsheet contains the following data:

Unit Serial Number	Cal Date	Cal Time	Cal Standard	Cal Temp in C	Check Date	Check Time	Check Standard	Check Result	Check Temp in C
90201895	12/29/2015	10:17 AM	0.16	21	01/27/2016	12:11 PM	0.08	0.081	20.8
90201895	12/29/2015	10:17 AM	0.16	21	01/27/2016	12:13 PM	0.08	0.08	21.3
90201895	12/29/2015	10:17 AM	0.16	21	02/18/2016	3:39 PM	0.08	0.04	22.8
90201895	12/29/2015	10:17 AM	0.16	21	03/08/2016	10:44 AM	0.08	0.045	24.6
90201895	12/29/2015	10:17 AM	0.16	21	04/01/2016	11:58 AM	0.08	0.08	23.8
90201895	12/29/2015	10:17 AM	0.16	21	04/01/2016	12:01 PM	0.08	0.08	24.3
90201895	12/29/2015	10:17 AM	0.16	21	04/04/2016	4:15 PM	0.08	0.077	22.5
90201895	12/29/2015	10:17 AM	0.16	21	04/04/2016	4:18 PM	0.08	0.074	22.8
90201895	12/29/2015	10:17 AM	0.16	21	04/06/2016	11:15 AM	0.08	0.077	23.6
90201895	12/29/2015	10:17 AM	0.16	21	04/06/2016	11:17 AM	0.08	0.077	24.1

Export can also save the data into different files such as excel or txt files and may be saved/printed out in that manner depending on the user preference. Note: Feel free to play around the settings tab to filter out data by serial number or set the file path where the data saves etc.

Property of Idaho State Police Internet Copy Forensic Services