




















Worklist: 7277

<u>LAB CASE</u>	<u>ITEM</u>	<u>ITEM TYPE</u>	<u>DESCRIPTION</u>	
P2025-3039	1	BCK	Alcohol Analysis	
P2025-3040	1	BCK	Alcohol Analysis	
P2025-3041	1	BCK	Alcohol Analysis	
P2025-3042	1	BCK	Alcohol Analysis	
P2025-3044	1	BCK	Alcohol Analysis	
P2025-3045	1	BCK	Alcohol Analysis	
P2025-3054	1	BCK	Alcohol Analysis	
P2025-3064	1	BCK	Alcohol Analysis	
P2025-3072	1	BCK	Alcohol Analysis	
P2025-3074	1	BCK	Alcohol Analysis	
P2025-3075	1	BCK	Alcohol Analysis	
P2025-3076	1	BCK	Alcohol Analysis	
P2025-3078	1	BCK	Alcohol Analysis	
P2025-3079	1	BCK	Alcohol Analysis	
P2025-3082	1	BCK	Alcohol Analysis	
P2025-3083	1	BCK	Alcohol Analysis	
P2025-3086	1	BCK	Alcohol Analysis	
P2025-3087	1	BCK	Alcohol Analysis	
P2025-3089	1	BCK	Alcohol Analysis	

AS

Quantitative Analysis for Ethanol & Qualitative Analysis for Other Volatiles

Analytical Method(s): 1.0

Device: Hamilton MICROLAB Liquid Processor/Dilutor Serial Number: ML600GB9897

Volatiles Quality Assurance Controls

Run Date(s): 10/08/2025

Calibration Date: (if different) 10/07/2025

Worklist #: 7277

Control level	Expiration	Lot #	Target Value	Acceptable Range	Overall Results
Level 1	Oct-26	2209047	0.0877	0.0789-0.0964	0.0798 g/100cc g/100cc g/100cc
Level 2	Mar-26	2110181	0.2030	0.1827-0.2233	0.1975 g/100cc 0.2102 g/100cc g/100cc
Multi-Component mixture: Curve Fit:			Exp: 2028 May	Lot # FN02162310	
		Column 1	0.99997	Column2	0.99993

Ethanol Calibration Reference Material

Calibrator level	Target Value	Acceptable Range	Column 1	Column 2	Precision	Mean
50	0.050	0.045 - 0.055	0.0507	0.0514	0.0007	0.051
100	0.100	0.090 - 0.110	0.1002	0.1002	0	0.1002
200	0.200	0.180 - 0.220	0.1991	0.1987	0.0004	0.1989
300	0.300	0.270 - 0.330	0.2988	0.2982	0.0006	0.2985
400	0.400	0.360 - 0.440	-	-	#####	#DIV/0!
500	0.500	0.450 - 0.550	0.5008	0.5013	0.0005	0.501

Aqueous Controls

Control level	Target Value	Acceptable Range	Overall Results
80	0.080	0.076 - 0.084	0.080 g/100cc



Internal Standard Monitoring Worksheet

Worksheet #:	7277	Run Date(s):	10/08/2025
---------------------	------	---------------------	------------

Internal Standard Solution:		Prep Date:	8/29/2025	Exp Date:	3/1/2026
------------------------------------	--	-------------------	-----------	------------------	----------

Sample Name	Column 1 Value	Column 2 Value
0.080	197869	193858
0.080	196823	192853
QC1	200739	196365
QC1	198866	194528
QC1		
QC1		
QC1		
QC1		
QC2	198454	194494
QC2	196879	192683
QC2	205047	200929
QC2	205253	201159
QC2		
QC2		


	Average	(-)20%	(+)20%
Column 1	199991.3	159993.0	239989.5
Column 2	195858.6	156686.9	235030.4



Calibration Table


Laboratory: Pocatello
 Instrument Name : GC SN- C12255850662 / HS SN- C12595700014

<<Data File>>
 Method File :Default Project - ALCOHOL_100725_TS.gcm
 Batch File :Default Project - BATCH_100725_TS.gcb
 Date Acquired :10/7/2025 11:40:52 AM
 Date Created :10/7/2025 11:37:25 AM
 Date Modified :10/9/2025 9:24:03 AM

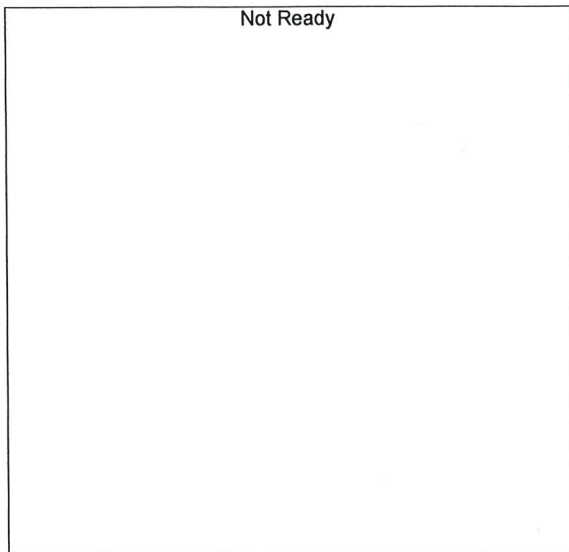

Name : METHANOL
 Detector Name: FID1
 Function : $f(x)=0*x+0$
 R^2 value= 0
 FitType: Linear
 ZeroThrough: Not Through


#	Conc.	Area	Std. Conc.	Data File Name
---	-------	------	------------	----------------

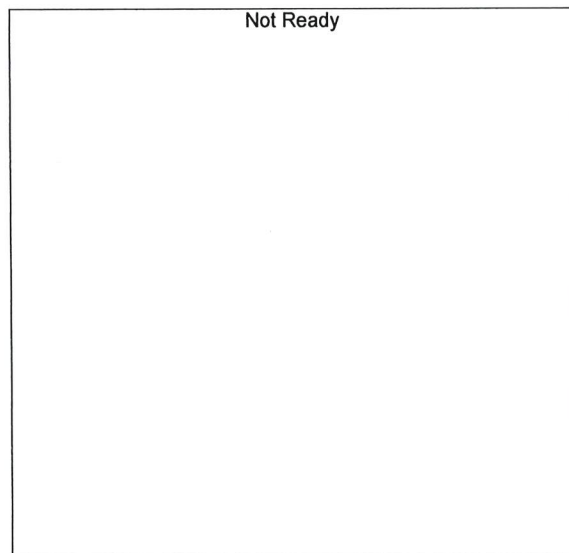

Name : ACETALDEHYDE
 Detector Name: FID1
 Function : $f(x)=0*x+0$
 R^2 value= 0
 FitType: Linear
 ZeroThrough: Not Through


#	Conc.	Area	Std. Conc.	Data File Name
---	-------	------	------------	----------------

TS

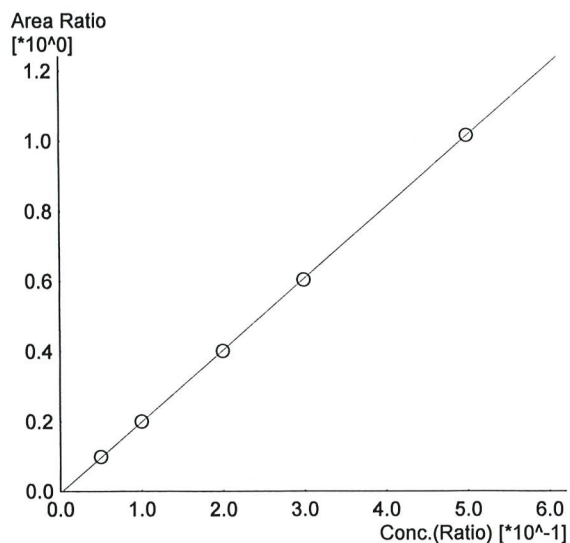


Name : ETHANOL
 Detector Name: FID1
 Function : $f(x)=2.03785*x-0.00483055$
 R² value= 0.9999735 ✓
 FitType: Linear
 ZeroThrough: Not Through

#	Conc.	Area	Std. Conc.	Data File Name
1	0.050	19369	0.0507	0.050_1072025_001.gcd
2	0.100	39088	0.1002	0.100_1072025_002.gcd
3	0.200	79885	0.1991	0.200_1072025_003.gcd
4	0.300	120375	0.2988	0.300_1072025_004.gcd
5	0.500	204331	0.5008	0.500_1072025_005.gcd

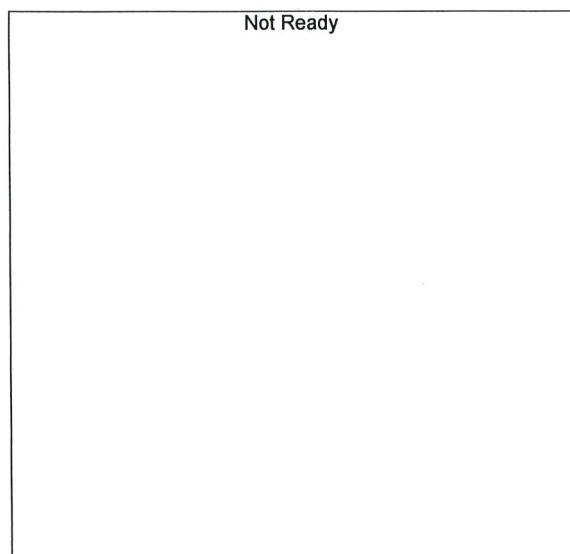

Name : ISOPROPYL ALCOHOL
 Detector Name: FID1
 Function : $f(x)=0*x+0$
 R² value= 0
 FitType: Linear
 ZeroThrough: Not Through


#	Conc.	Area	Std. Conc.	Data File Name
---	-------	------	------------	----------------

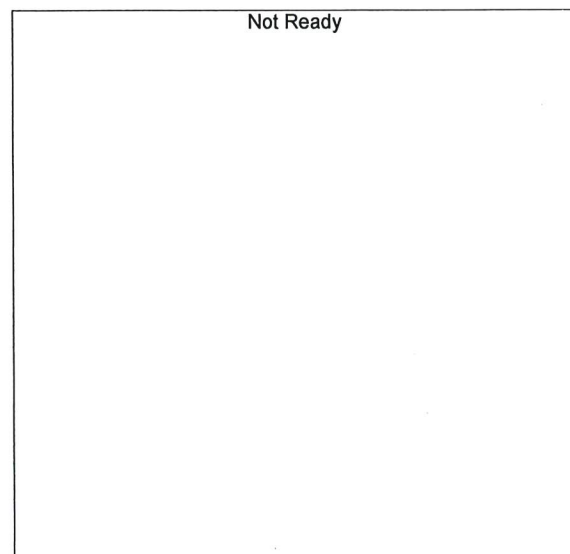

Name : ACETONE
 Detector Name: FID1
 Function : $f(x)=0*x+0$
 R² value= 0
 FitType: Linear
 ZeroThrough: Not Through

#	Conc.	Area	Std. Conc.	Data File Name
---	-------	------	------------	----------------

B

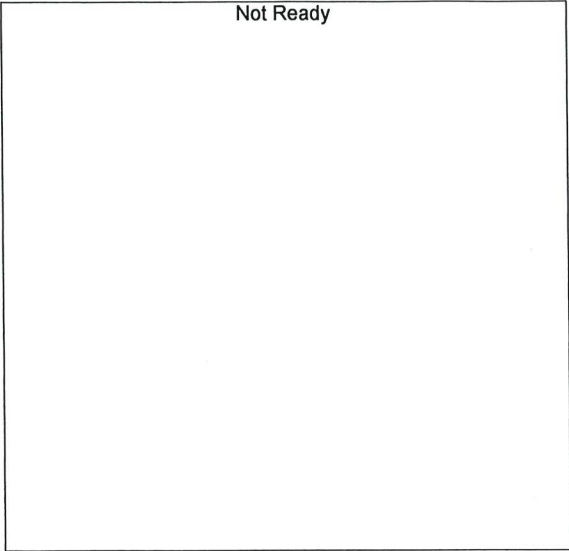


Name : DFE/TFE
Detector Name: FID1
Function : $f(x)=0*x+0$
R^2 value= 0
FitType: Linear
ZeroThrough: Not Through

#	Conc.	Area	Std. Conc.	Data File Name
---	-------	------	------------	----------------




Name : DME
Detector Name: FID1
Function : $f(x)=0*x+0$
R^2 value= 0
FitType: Linear
ZeroThrough: Not Through

#	Conc.	Area	Std. Conc.	Data File Name
---	-------	------	------------	----------------

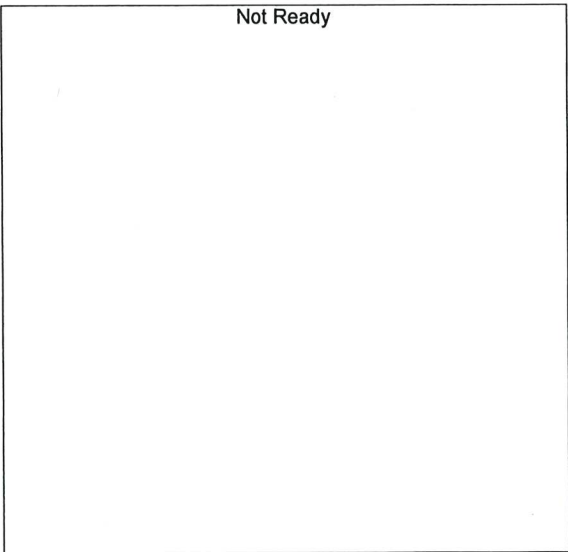


Name : ACETALDEHYDE
Detector Name: FID2
Function : $f(x)=0*x+0$
R^2 value= 0
FitType: Linear
ZeroThrough: Not Through

#	Conc.	Area	Std. Conc.	Data File Name
---	-------	------	------------	----------------

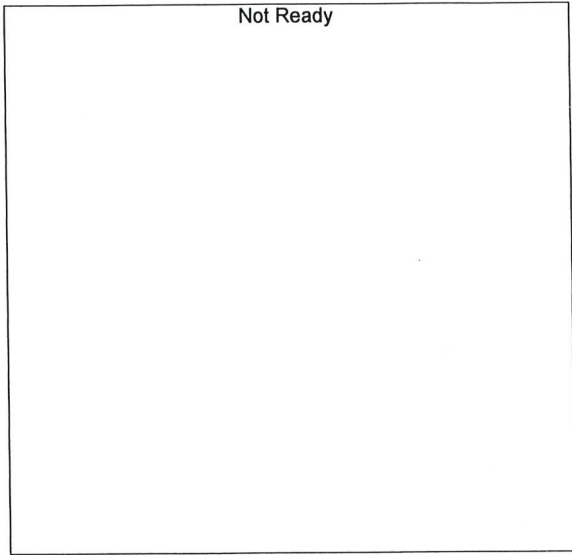


Name : METHANOL
 Detector Name: FID2
 Function : $f(x)=0*x+0$
 R² value= 0
 FitType: Linear
 ZeroThrough: Not Through

#	Conc.	Area	Std. Conc.	Data File Name
---	-------	------	------------	----------------

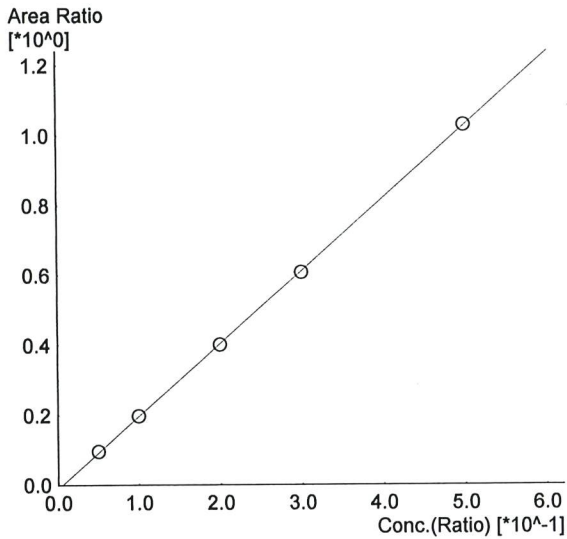

Name : ETHANOL
 Detector Name: FID2
 Function : $f(x)=2.07322*x-0.0110243$
 R² value= 0.9999331 ✓
 FitType: Linear
 ZeroThrough: Not Through


#	Conc.	Area	Std. Conc.	Data File Name
1	0.050	18250	0.0514	0.050_1072025_001.gcd
2	0.100	37446	0.1002	0.100_1072025_002.gcd
3	0.200	77807	0.1987	0.200_1072025_003.gcd
4	0.300	118117	0.2982	0.300_1072025_004.gcd
5	0.500	202578	0.5013	0.500_1072025_005.gcd

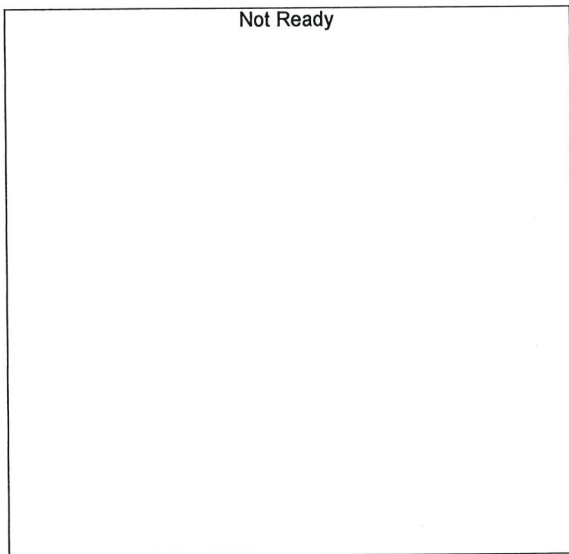

Name : ACETONE
 Detector Name: FID2
 Function : $f(x)=0*x+0$
 R² value= 0
 FitType: Linear
 ZeroThrough: Not Through


#	Conc.	Area	Std. Conc.	Data File Name
---	-------	------	------------	----------------

10

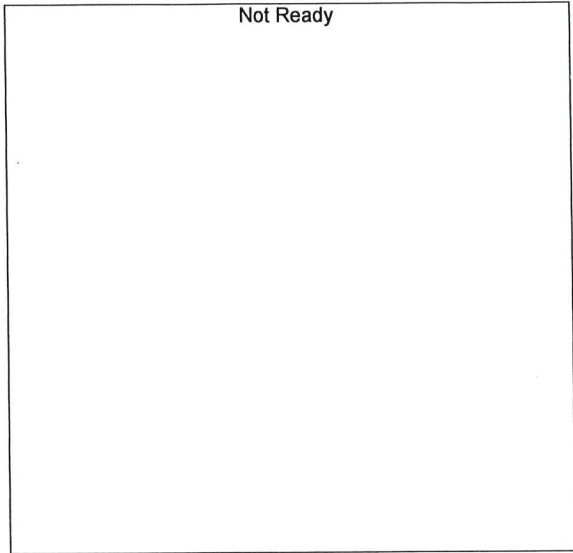


Name : ISOPROPYL ALCOHOL
Detector Name: FID2
Function : $f(x)=0*x+0$
R^2 value= 0
FitType: Linear
ZeroThrough: Not Through

#	Conc.	Area	Std. Conc.	Data File Name
---	-------	------	------------	----------------

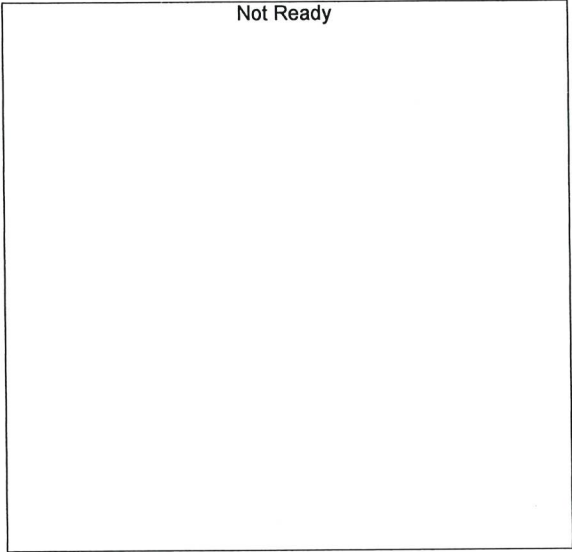

Name : DFE
Detector Name: FID2
Function : $f(x)=0*x+0$
R^2 value= 0
FitType: Linear
ZeroThrough: Not Through



#	Conc.	Area	Std. Conc.	Data File Name
---	-------	------	------------	----------------

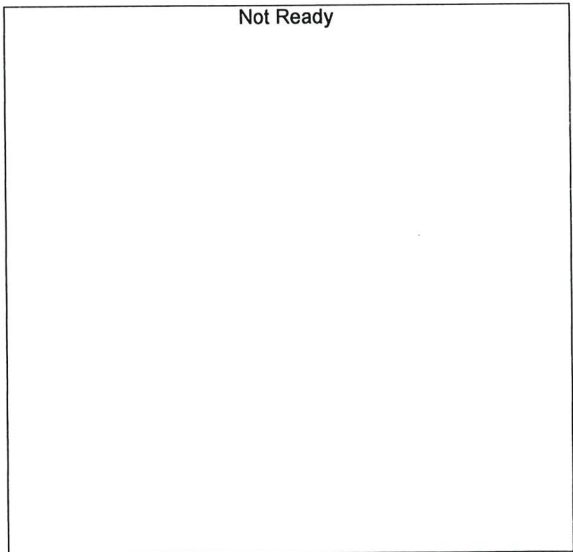

Name : TFE
Detector Name: FID2
Function : $f(x)=0*x+0$
R^2 value= 0
FitType: Linear
ZeroThrough: Not Through

#	Conc.	Area	Std. Conc.	Data File Name
---	-------	------	------------	----------------

Sample Name : 0.050
 Vial # : 1
 Data Filename : 0.050_1072025_001.gcd
 Method Filename : ALCOHOL_100725_TS.gcm
 Batch Filename : BATCH_100725_TS.gcb
 Date Acquired : 10/7/2025 11:02:45 AM
 Date Processed : 10/9/2025 9:23:50 AM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

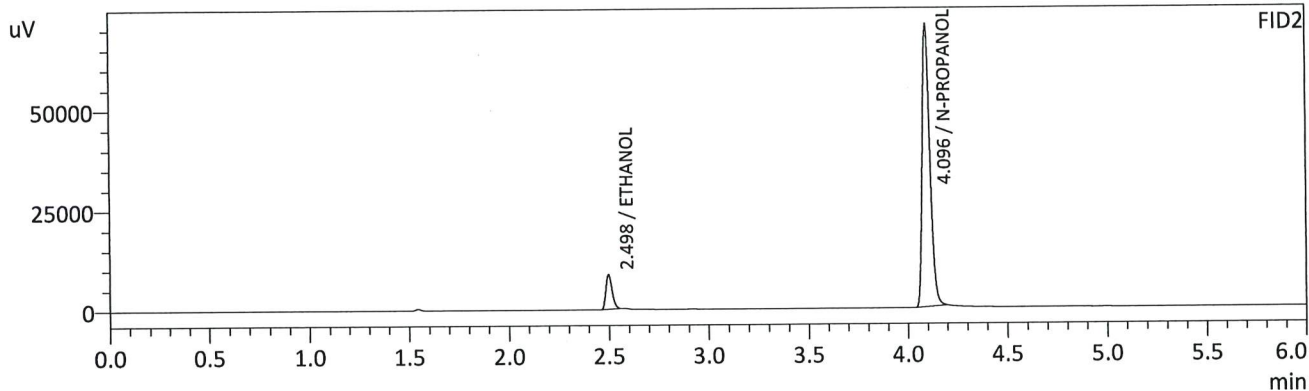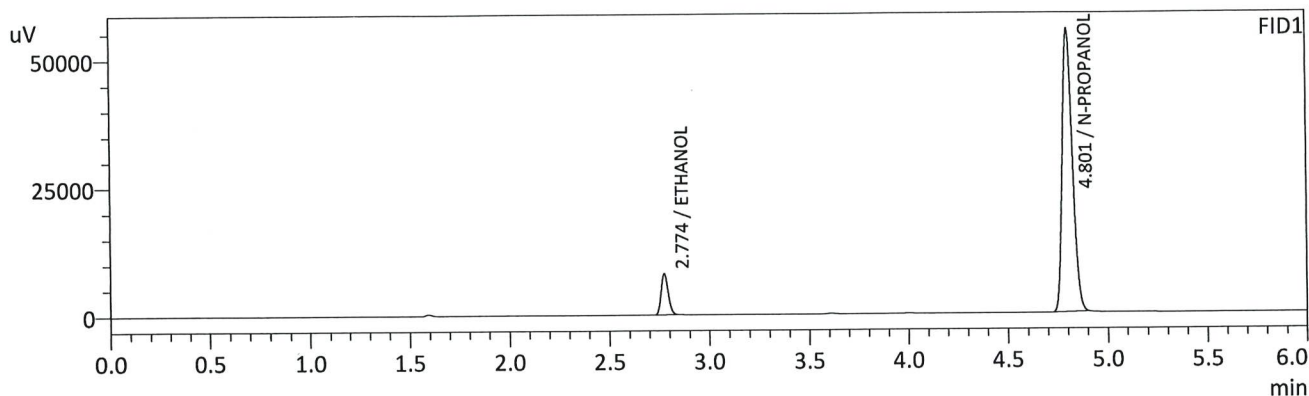

FID1



Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	0.0507	g/100cc	19369	7959
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	196306	55212
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	0.0514	g/100cc	18250	8616
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	191021	70503
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

15

Sample Name : 0.100
 Vial # : 2
 Data Filename : 0.100_1072025_002.gcd
 Method Filename : ALCOHOL_100725_TS.gcm
 Batch Filename : BATCH_100725_TS.gcb
 Date Acquired : 10/7/2025 11:12:15 AM
 Date Processed : 10/9/2025 9:23:53 AM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

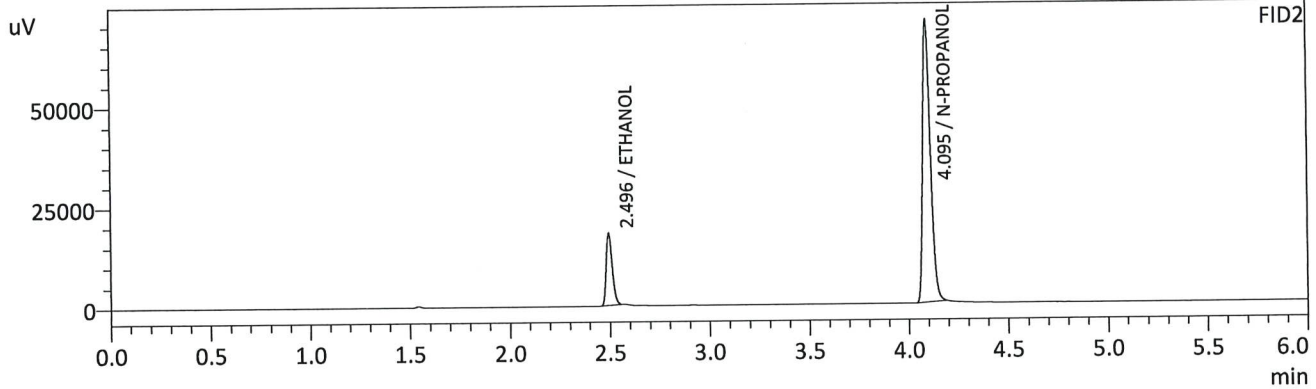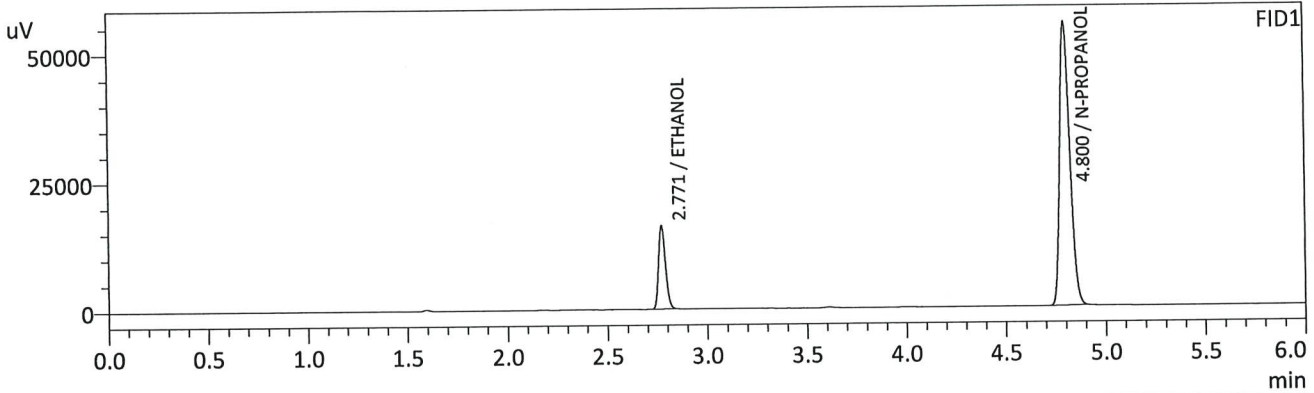

FID1



Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	0.1002	g/100cc	39088	16141
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	195878	55164
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	0.1002	g/100cc	37446	17908
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	190234	70271
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

10

Sample Name : 0.200
 Vial # : 3
 Data Filename : 0.200_1072025_003.gcd
 Method Filename : ALCOHOL_100725_TS.gcm
 Batch Filename : BATCH_100725_TS.gcb
 Date Acquired : 10/7/2025 11:21:37 AM
 Date Processed : 10/9/2025 9:23:57 AM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

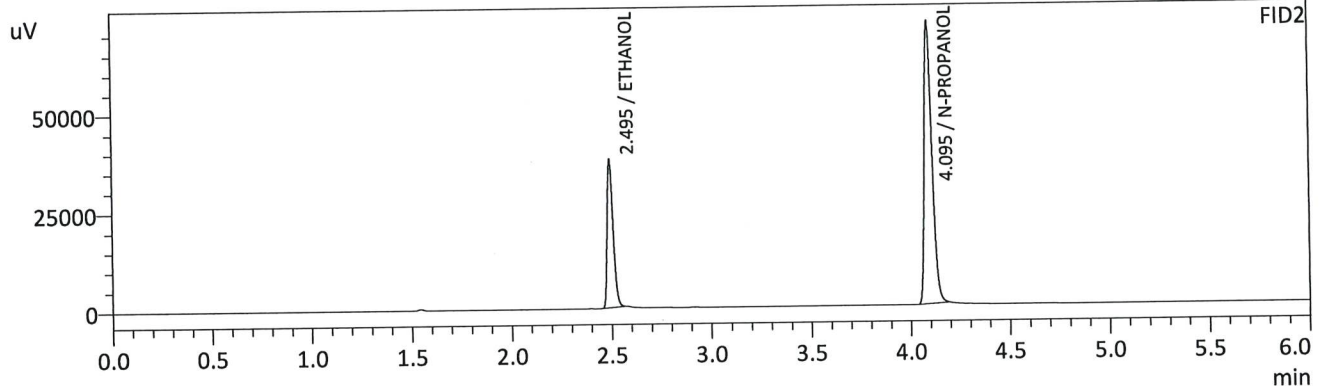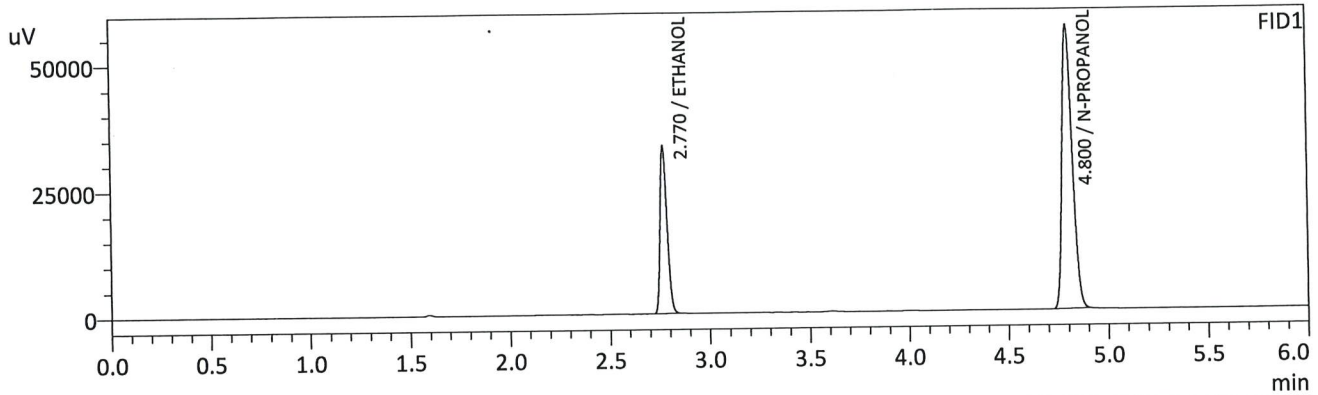

FID1



Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	0.1991	g/100cc	79885	33197
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	199194	56235
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	0.1987	g/100cc	77807	37586
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	194065	71731
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

TS

Sample Name : 0.300
 Vial # : 4
 Data Filename : 0.300_1072025_004.gcd
 Method Filename : ALCOHOL_100725_TS.gcm
 Batch Filename : BATCH_100725_TS.gcb
 Date Acquired : 10/7/2025 11:31:22 AM
 Date Processed : 10/9/2025 9:24:00 AM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

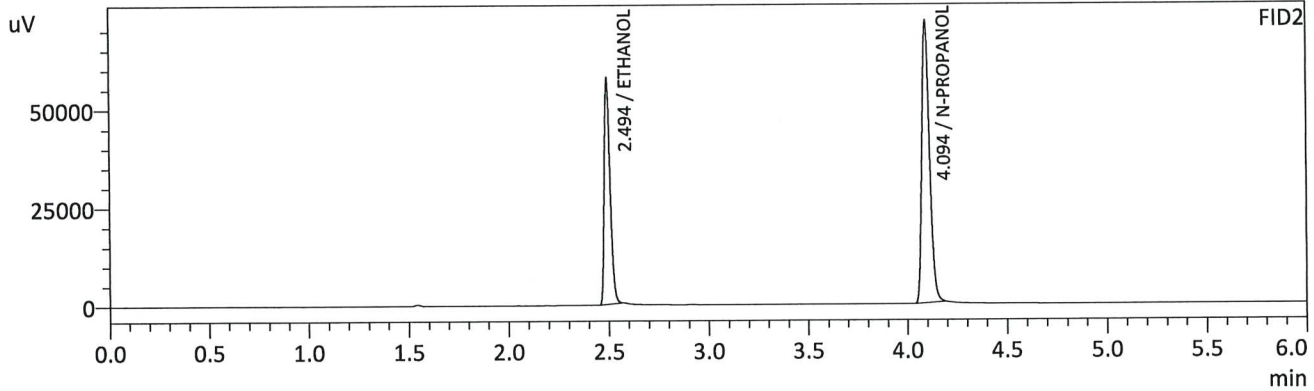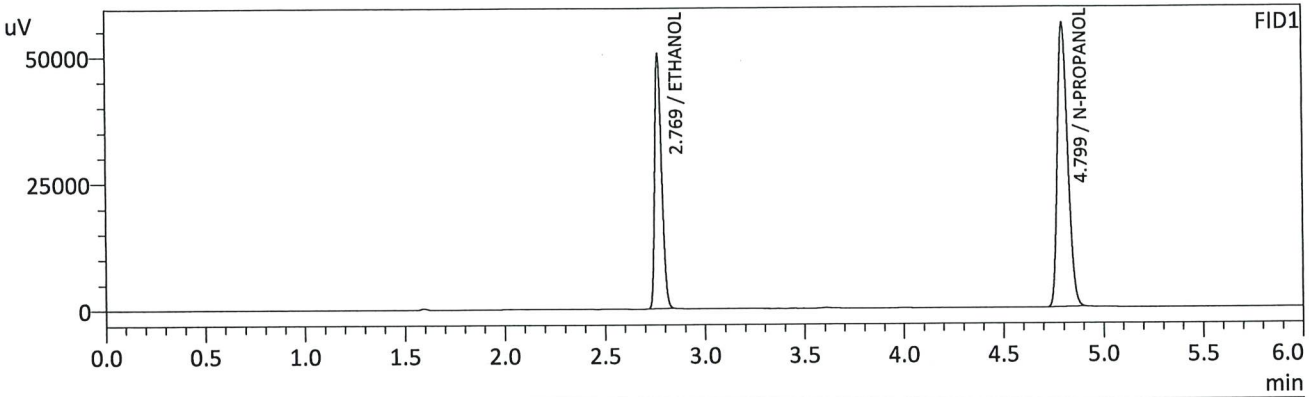

FID1



Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	0.2988	g/100cc	120375	50177
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	199212	56079
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	0.2982	g/100cc	118117	57365
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	194478	71678
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

TS

Sample Name : 0.500
 Vial # : 5
 Data Filename : 0.500_1072025_005.gcd
 Method Filename : ALCOHOL_100725_TS.gcm
 Batch Filename : BATCH_100725_TS.gcb
 Date Acquired : 10/7/2025 11:40:52 AM
 Date Processed : 10/9/2025 9:24:03 AM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

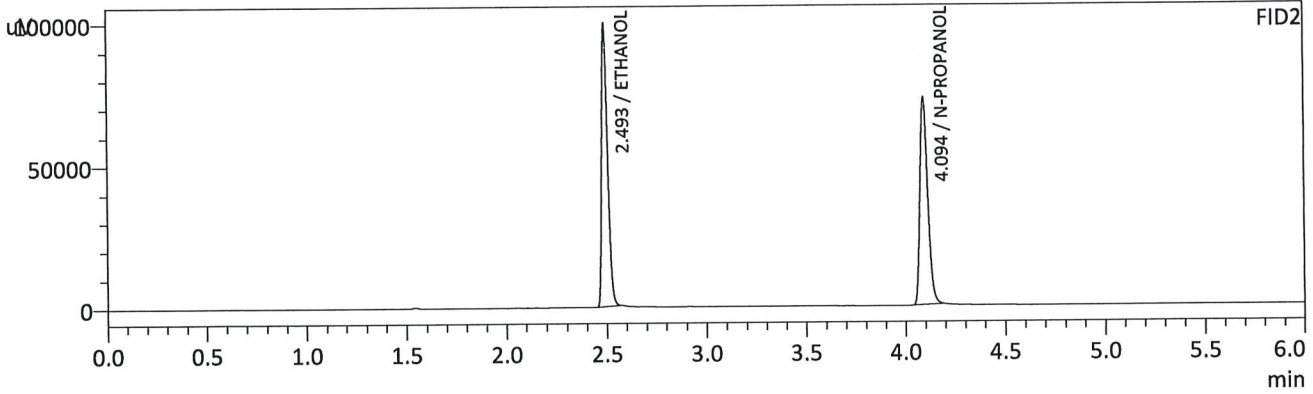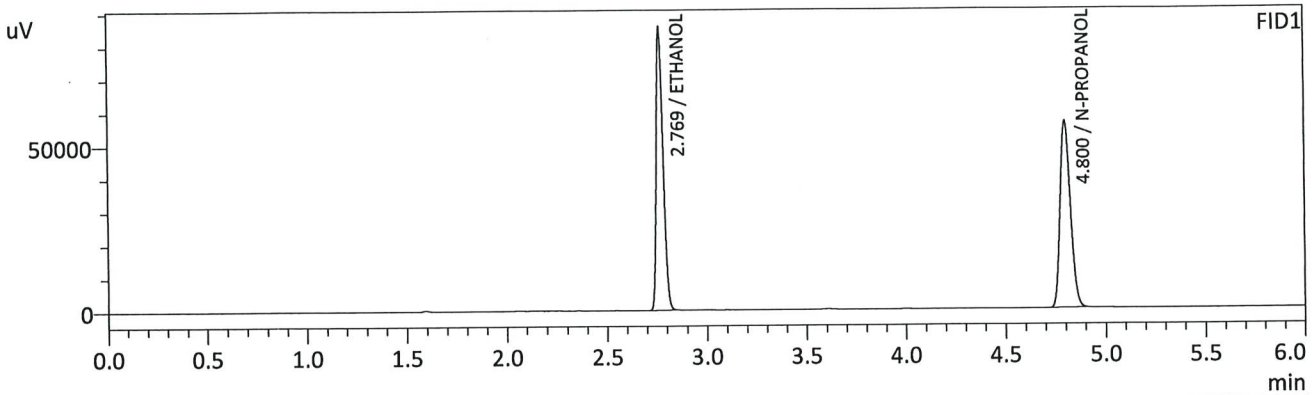

FID1



Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	0.5008	g/100cc	204331	85172
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	201142	56524
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	0.5013	g/100cc	202578	98676
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	196980	72712
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

TS

Sample Name : INT STD BLK 1
 Vial # : 1
 Data Filename : INT STD BLK 1_1082025_001.gcd
 Method Filename : ALCOHOL_100725_TS.gcm
 Batch Filename : BATCH_100825_TS.gcb
 Date Acquired : 10/8/2025 10:53:54 AM
 Date Processed : 10/8/2025 10:59:54 AM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

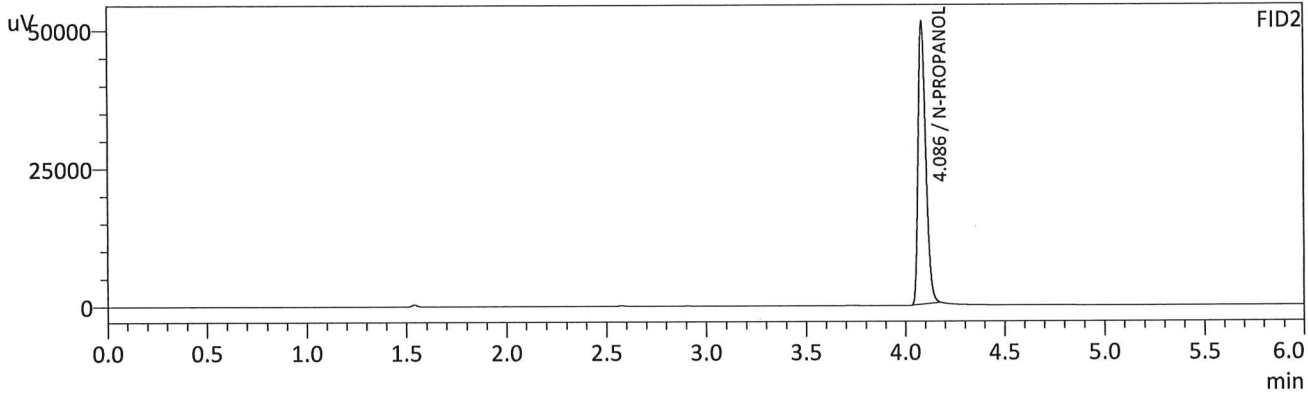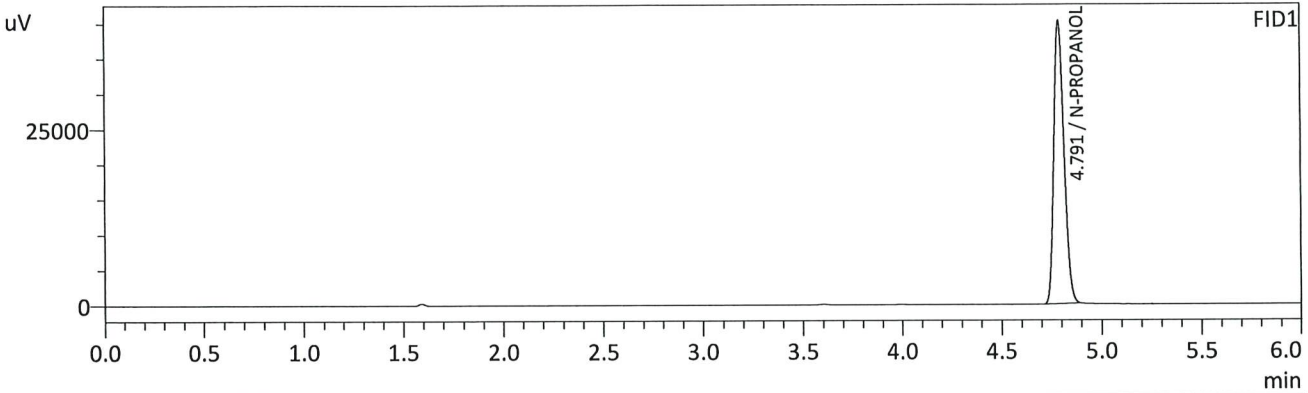

FID1



Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	142419	40185
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	138093	51254
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

TS

Sample Name : MULTI-COMP MIX
 Vial # : 2
 Data Filename : MULTI-COMP MIX_1082025_002.gcd
 Method Filename : ALCOHOL_100725_TS.gcm
 Batch Filename : BATCH_100825_TS.gcb
 Date Acquired : 10/8/2025 11:03:23 AM
 Date Processed : 10/8/2025 11:09:25 AM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

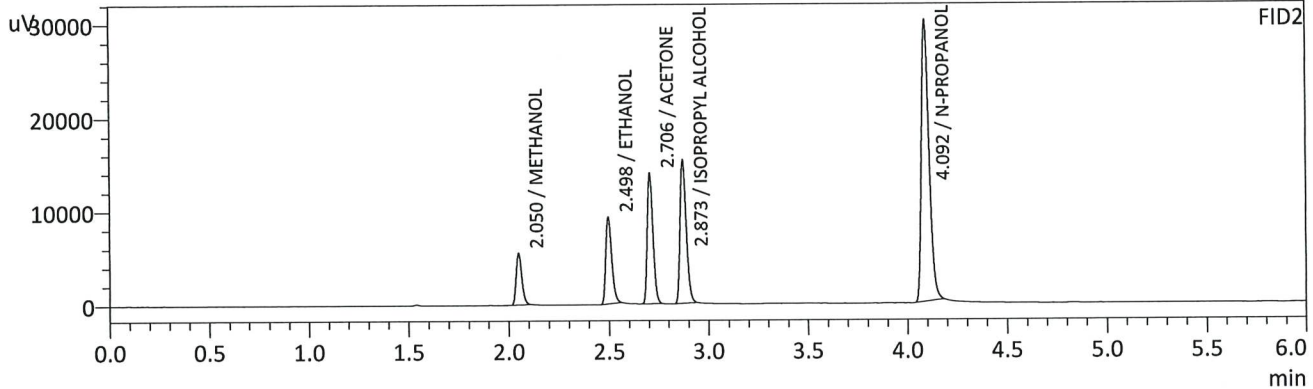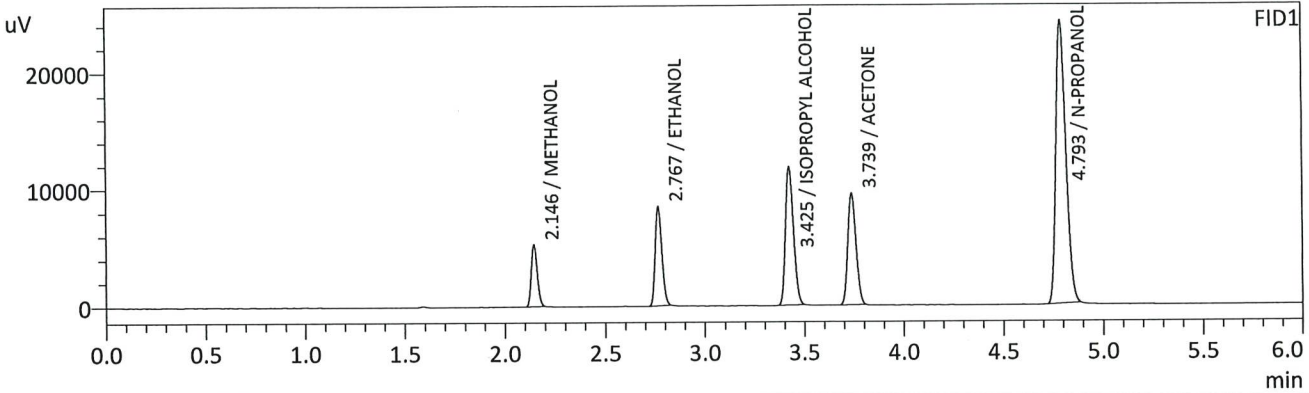

FID1



Name	Conc.	Unit	Area	Height
METHANOL	0.0000	g/100cc	10993	5241
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	0.1175	g/100cc	19845	8402
ISOPROPYL ALCOHOL	0.0000	g/100cc	33043	11734
ACETONE	0.0000	g/100cc	27261	9449
N-PROPANOL	0.0000	g/100cc	84512	24120
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	0.0000	g/100cc	10773	5484
ETHANOL	0.1183	g/100cc	18838	9119
ACETONE	0.0000	g/100cc	28083	13850
ISOPROPYL ALCOHOL	0.0000	g/100cc	32690	15271
N-PROPANOL	0.0000	g/100cc	80416	30010
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

TS

Sample Name : INT STD BLK 2
 Vial # : 3
 Data Filename : INT STD BLK 2_1082025_003.gcd
 Method Filename : ALCOHOL_100725_TS.gcm
 Batch Filename : BATCH_100825_TS.gcb
 Date Acquired : 10/8/2025 11:12:45 AM
 Date Processed : 10/8/2025 11:18:47 AM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

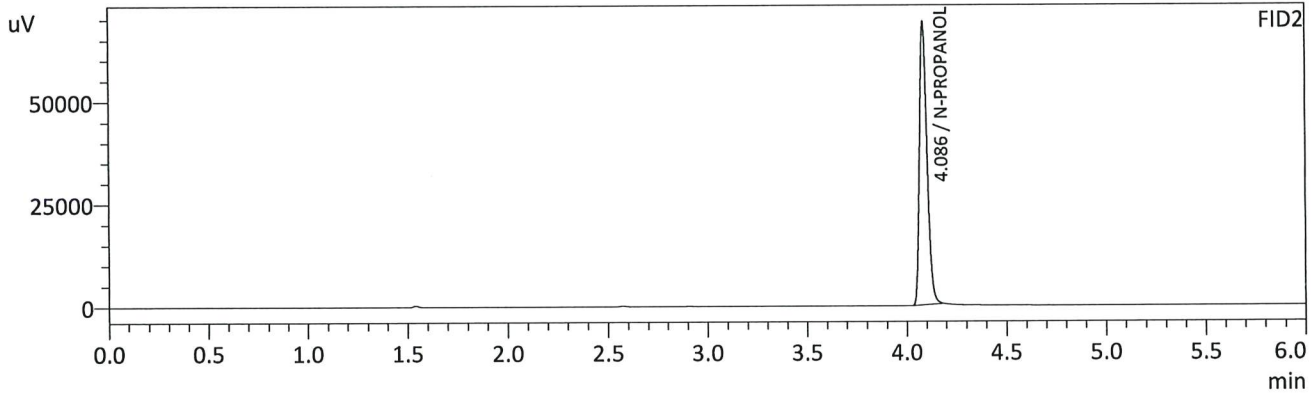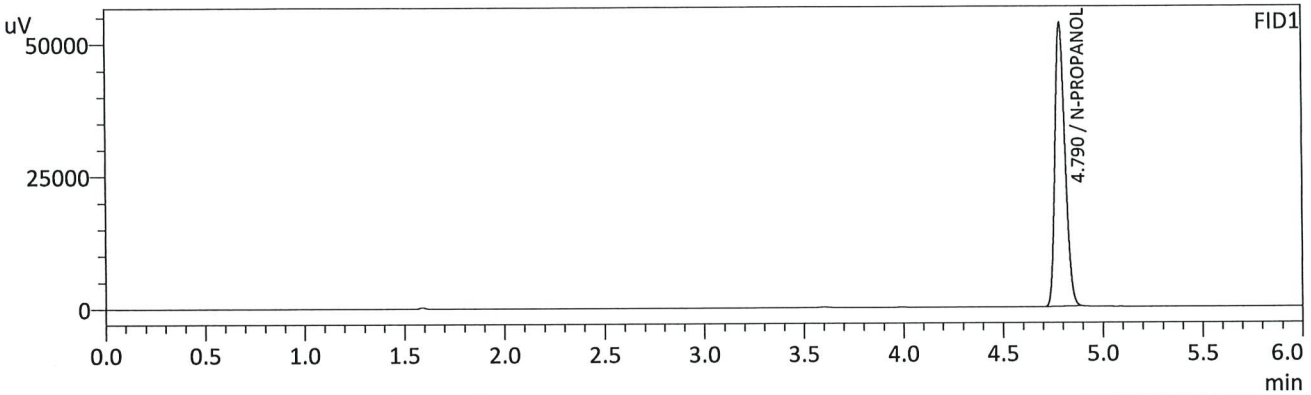

FID1

Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	189990	53552
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	185136	68934
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

15

VOLATILES DETERMINATION CASEFILE WORKSHEET

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No: 0.08 QA		Analysis Date(s): 10/8/2025 11:41:18 AM(-06:00)				
	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Sample A-B Difference	Over-all Mean
Sample Results	0.0805	0.0806	0.0001	0.0805	0.0000	0.0805
(g/100cc)	0.0806	0.0805	0.0001	0.0805		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument information is stored centrally.

Refer To Instrument Method: ALCOHOL_100725_TS.gcm



Reporting of Results	Uncertainty of Measurements (UM%): 5.00%		
Overall Mean (g/100cc)	Low	High	5 % of Mean
0.080	0.076	0.084	0.004

Reported Results	
0.080	

Calibration and control data are stored centrally.

15

Sample Name : 0.08 QA
 Vial # : 6
 Data Filename : 0.08 QA_1082025_006.gcd
 Method Filename : ALCOHOL_100725_TS.gcm
 Batch Filename : BATCH_100825_TS.gcb
 Date Acquired : 10/8/2025 11:41:18 AM
 Date Processed : 10/8/2025 11:47:20 AM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

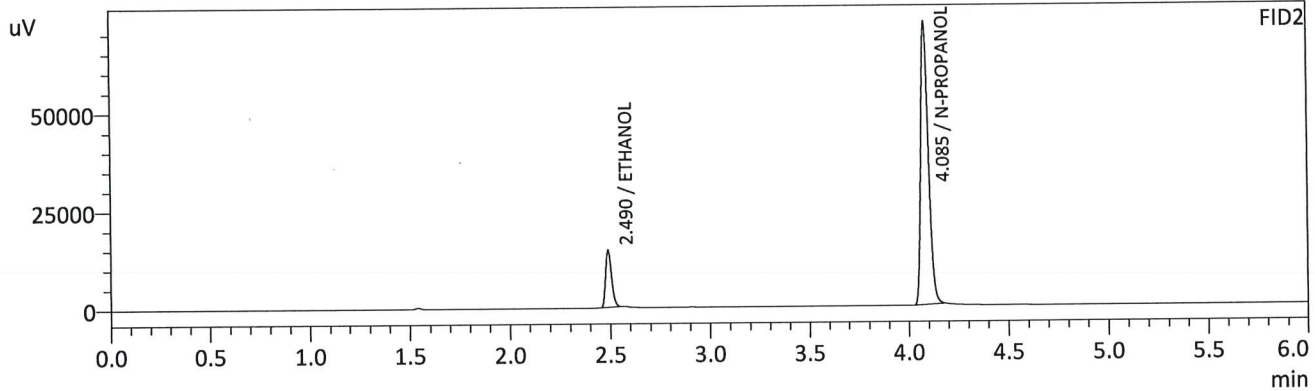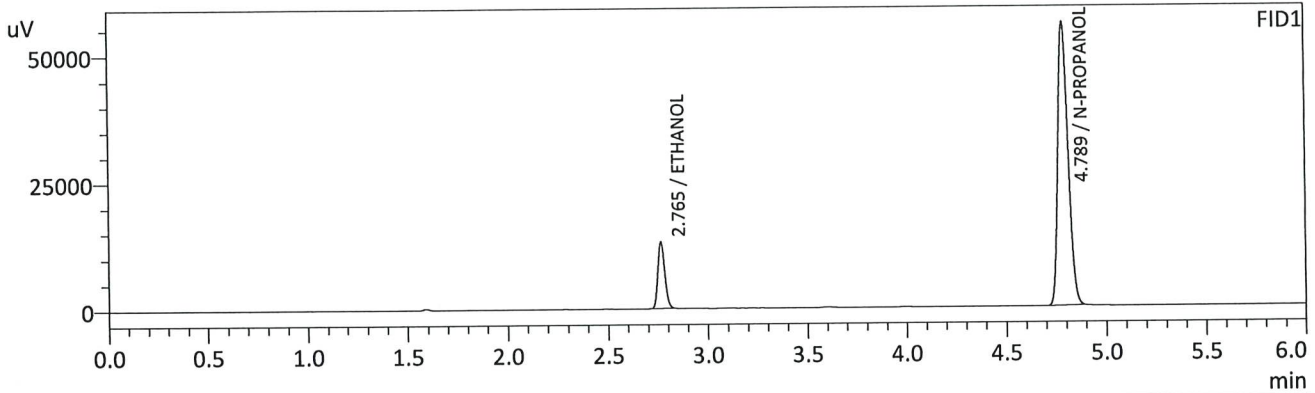

FID1



Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	0.0805	g/100cc	31531	13076
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	197869	55614
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	0.0806	g/100cc	30269	14563
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	193858	71913
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

TS

Sample Name : 0.08 QA - B
 Vial # : 7
 Data Filename : 0.08 QA - B_1082025_007.gcd
 Method Filename : ALCOHOL_100725_TS.gcm
 Batch Filename : BATCH_100825_TS.gcb
 Date Acquired : 10/8/2025 11:51:02 AM
 Date Processed : 10/8/2025 11:57:04 AM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

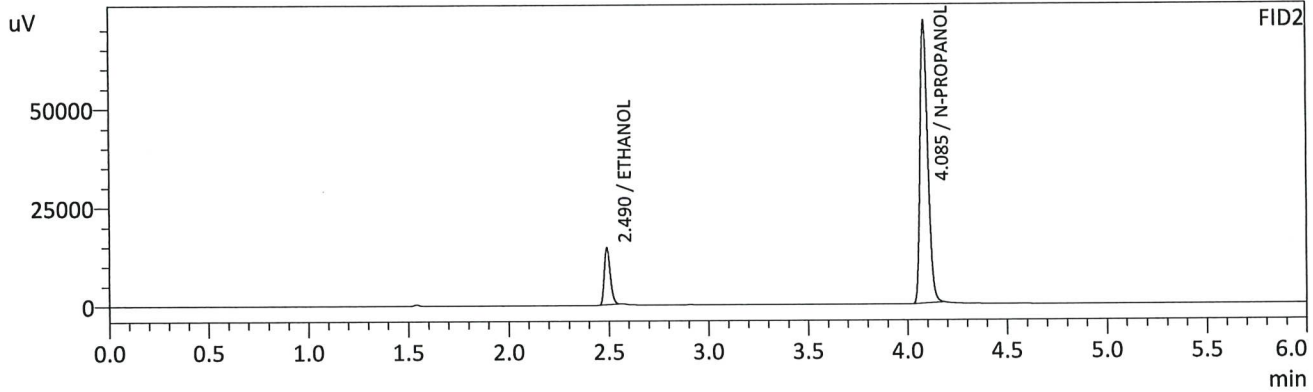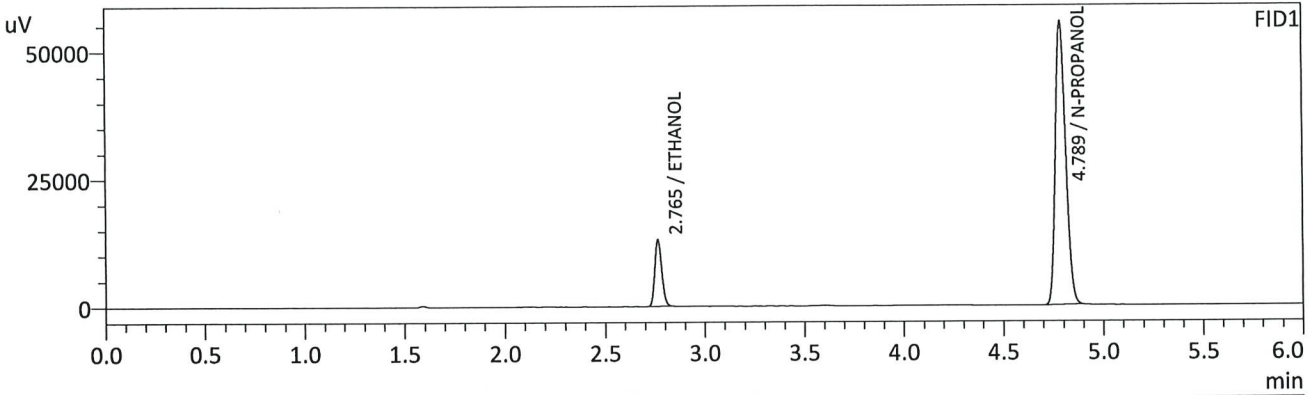

FID1

Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	0.0806	g/100cc	31378	13030
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	196823	55446
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	0.0805	g/100cc	30096	14478
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	192853	71511
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

B

VOLATILES DETERMINATION CASEFILE WORKSHEET

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No: QC1-1		Analysis Date(s): 10/8/2025 11:22:29 AM(-06:00)				
	Column 1	Column 2	Column	Mean	Sample A-B	Over-all Mean
	FID A	FID B	Precision	Value	Difference	
Sample Results	0.0798	0.0799	0.0001	0.0798	0.0000	0.0798
(g/100cc)	0.0798	0.0799	0.0001	0.0798		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument information is stored centrally.

Refer To Instrument Method: ALCOHOL_100725_TS.gcm



Reporting of Results	Uncertainty of Measurements (UM%): 5.00%		
Overall Mean (g/100cc)	Low	High	5 % of Mean
0.079	0.075	0.083	0.004

Reported Results	
0.079	

Calibration and control data are stored centrally.

15

Sample Name : QC1-1
 Vial # : 4
 Data Filename : QC1-1_1082025_004.gcd
 Method Filename : ALCOHOL_100725_TS.gcm
 Batch Filename : BATCH_100825_TS.gcb
 Date Acquired : 10/8/2025 11:22:29 AM
 Date Processed : 10/8/2025 11:28:31 AM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

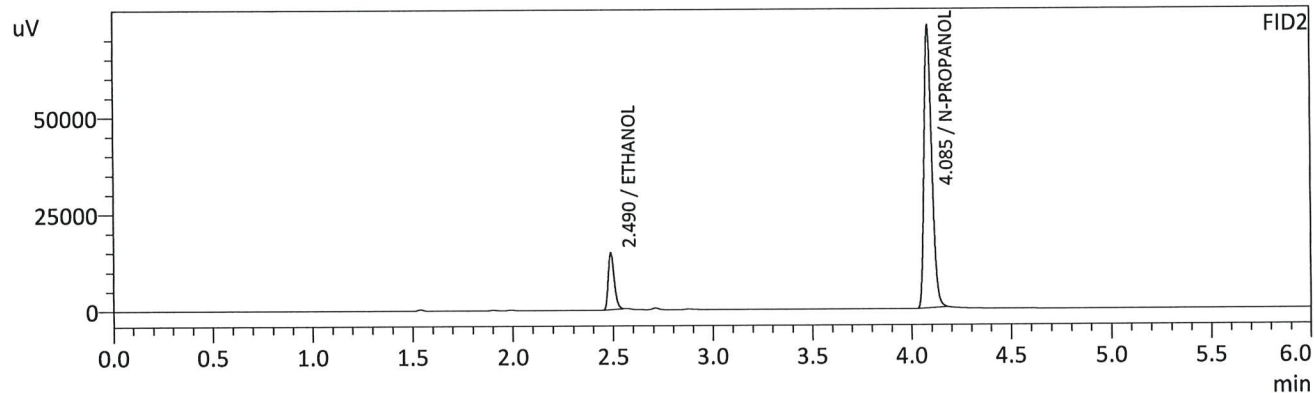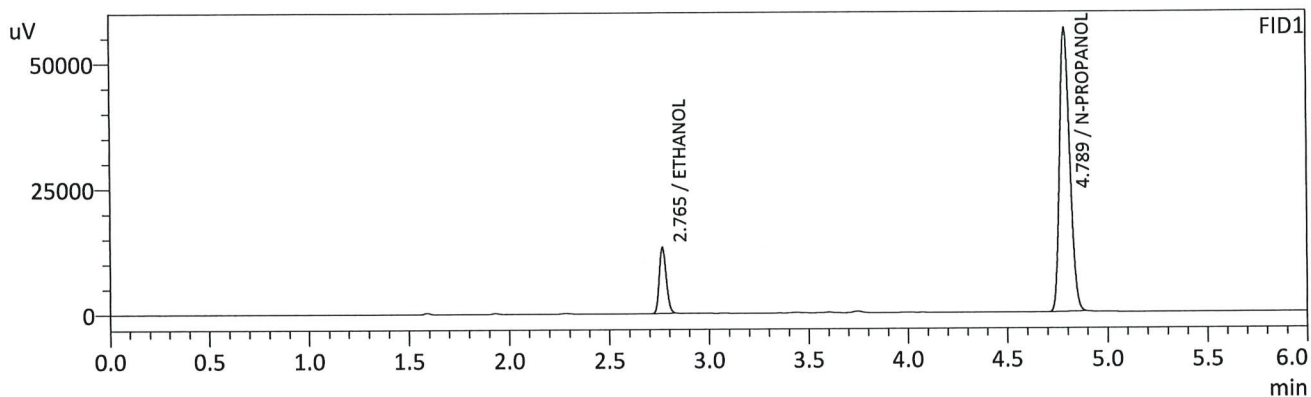

FID1



Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	0.0798	g/100cc	31697	13142
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	200739	56503
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	0.0799	g/100cc	30388	14606
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	196365	73001
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

TS

Sample Name : QC1-1-B
 Vial # : 5
 Data Filename : QC1-1-B_1082025_005.gcd
 Method Filename : ALCOHOL_100725_TS.gcm
 Batch Filename : BATCH_100825_TS.gcb
 Date Acquired : 10/8/2025 11:32:00 AM
 Date Processed : 10/8/2025 11:38:02 AM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

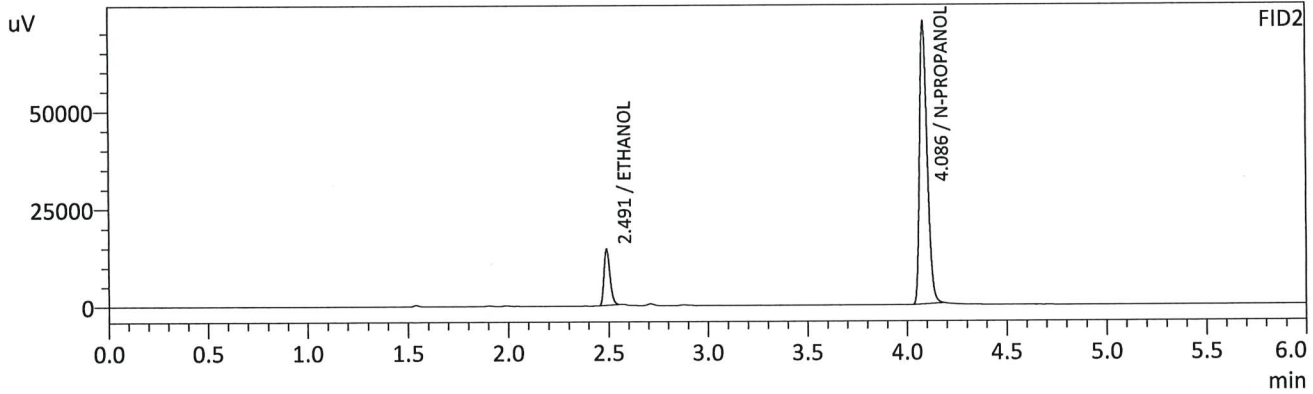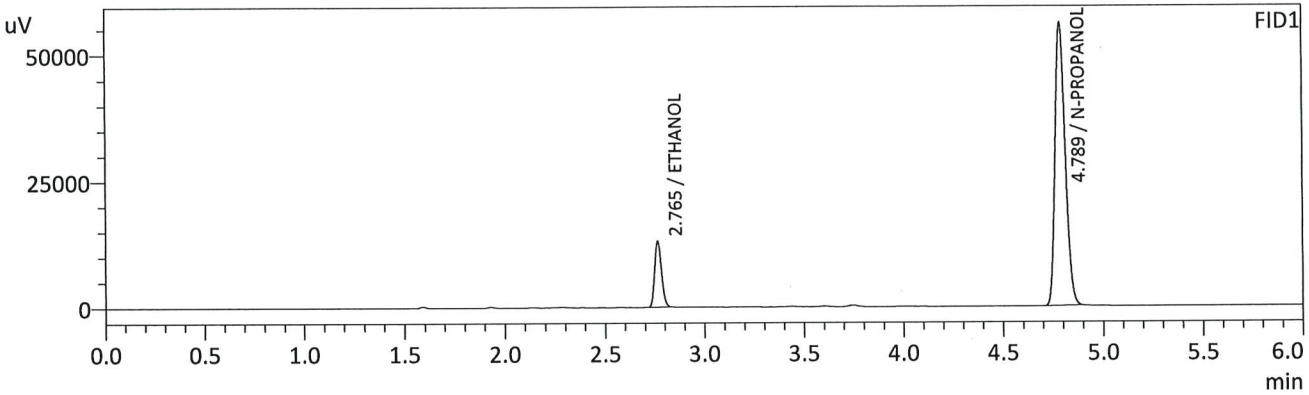

FID1

Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	0.0798	g/100cc	31387	13032
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	198866	56018
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	0.0799	g/100cc	30109	14475
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	194528	72400
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

15

VOLATILES DETERMINATION CASEFILE WORKSHEET

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No: QC2-1		Analysis Date(s): 10/8/2025 2:52:01 PM(-06:00)				
	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Sample A-B Difference	Over-all Mean
Sample Results	0.1973	0.1968	0.0005	0.1970	0.0010	0.1975
(g/100cc)	0.1982	0.1978	0.0004	0.1980		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument information is stored centrally.

Refer To Instrument Method: ALCOHOL_100725_TS.gcm



Reporting of Results	Uncertainty of Measurements (UM%): 5.00%		
Overall Mean (g/100cc)	Low	High	5 % of Mean
0.197	0.187	0.207	0.010

Reported Results	
0.197	

Calibration and control data are stored centrally.

15

Sample Name : QC2-1
 Vial # : 26
 Data Filename : QC2-1_1082025_026.gcd
 Method Filename : ALCOHOL_100725_TS.gcm
 Batch Filename : BATCH_100825_TS.gcb
 Date Acquired : 10/8/2025 2:52:01 PM
 Date Processed : 10/8/2025 2:58:01 PM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

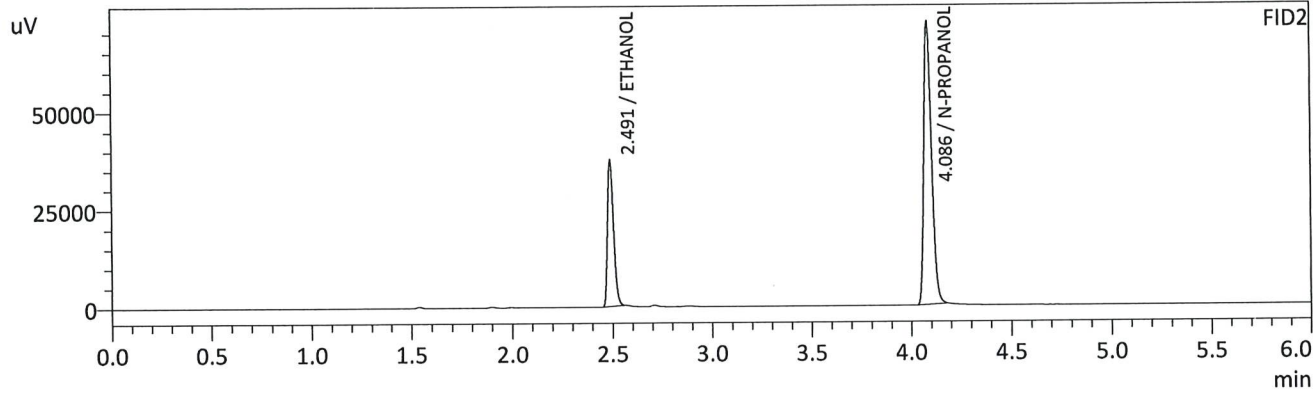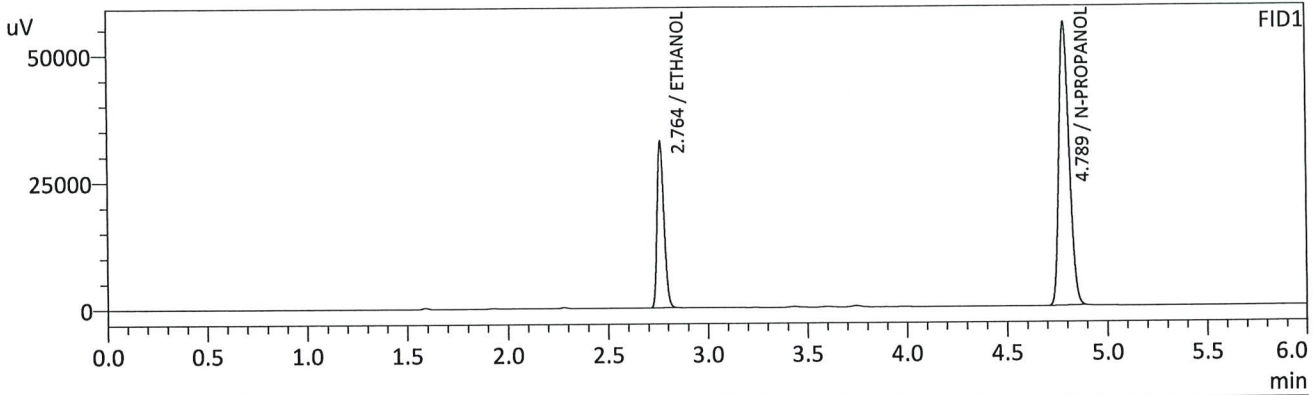

FID1



Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	0.1973	g/100cc	78865	32494
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	198454	55693
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	0.1968	g/100cc	77219	37217
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	194494	72182
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

TS

Sample Name : QC2-1-B
 Vial # : 27
 Data Filename : QC2-1-B_1082025_027.gcd
 Method Filename : ALCOHOL_100725_TS.gcm
 Batch Filename : BATCH_100825_TS.gcb
 Date Acquired : 10/8/2025 3:01:17 PM
 Date Processed : 10/8/2025 3:07:19 PM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

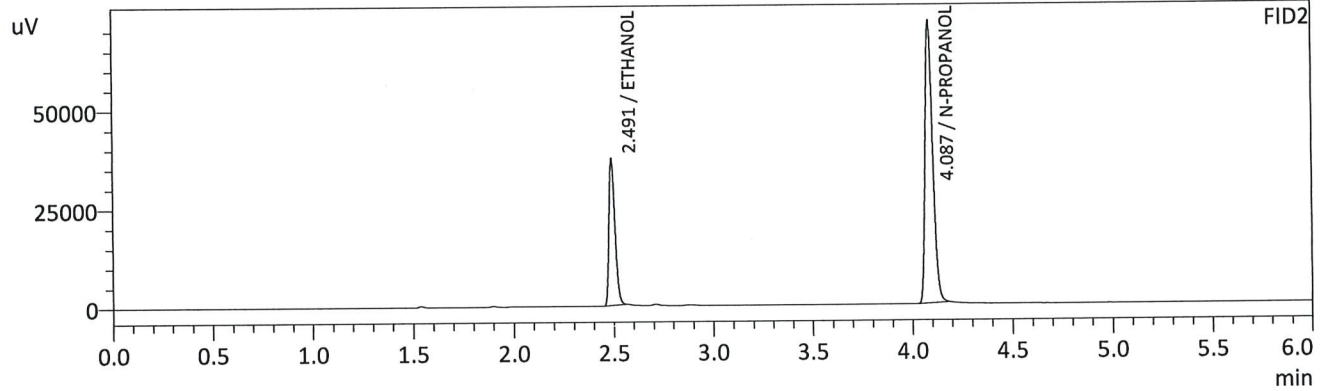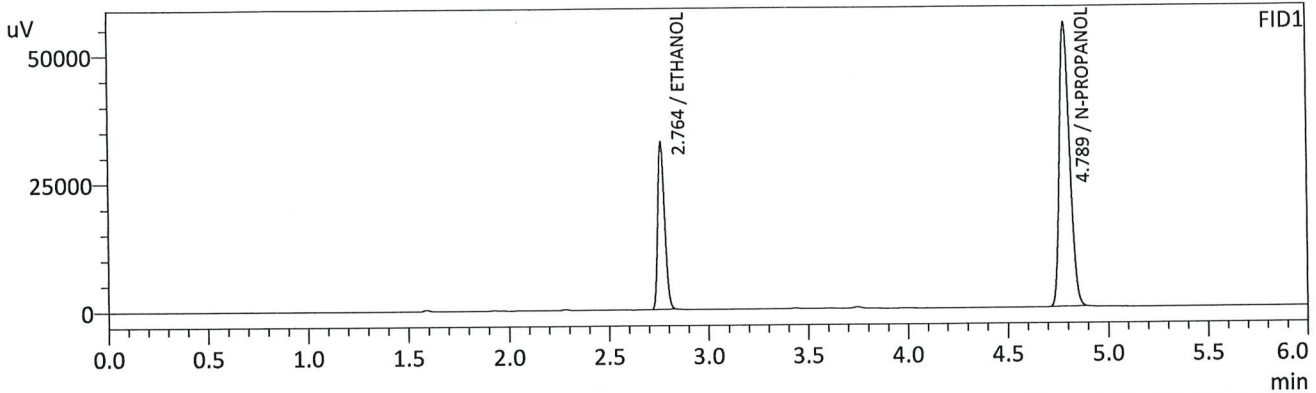

FID1

Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	0.1982	g/100cc	78607	32474
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	196879	55410
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	0.1978	g/100cc	76920	36960
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	192683	71494
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

TS

VOLATILES DETERMINATION CASEFILE WORKSHEET

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No: QC2-2		Analysis Date(s): 10/8/2025 6:21:23 PM(-06:00)				
	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Sample A-B Difference	Over-all Mean
Sample Results	0.2105	0.2106	0.0001	0.2105	0.0005	0.2102
(g/100cc)	0.2101	0.2099	0.0002	0.2100		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument information is stored centrally.

Refer To Instrument Method: ALCOHOL_100725_TS.gcm



Reporting of Results	Uncertainty of Measurements (UM%): 5.00%		
Overall Mean (g/100cc)	Low	High	5 % of Mean
0.210	0.199	0.221	0.011

Reported Results	
0.210	

Calibration and control data are stored centrally.

TS

Sample Name : QC2-2
 Vial # : 48
 Data Filename : QC2-2_1082025_048.gcd
 Method Filename : ALCOHOL_100725_TS.gcm
 Batch Filename : BATCH_100825_TS.gcb
 Date Acquired : 10/8/2025 6:21:23 PM
 Date Processed : 10/9/2025 7:57:00 AM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

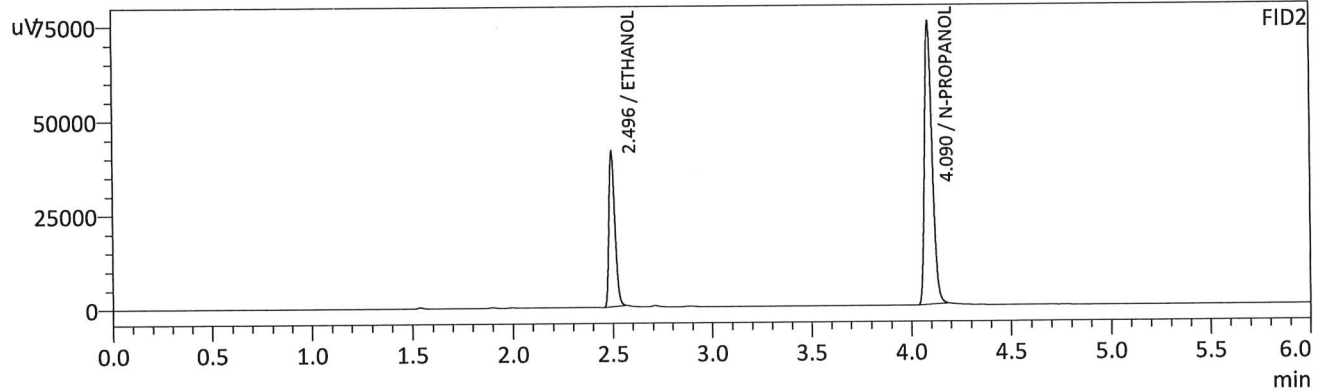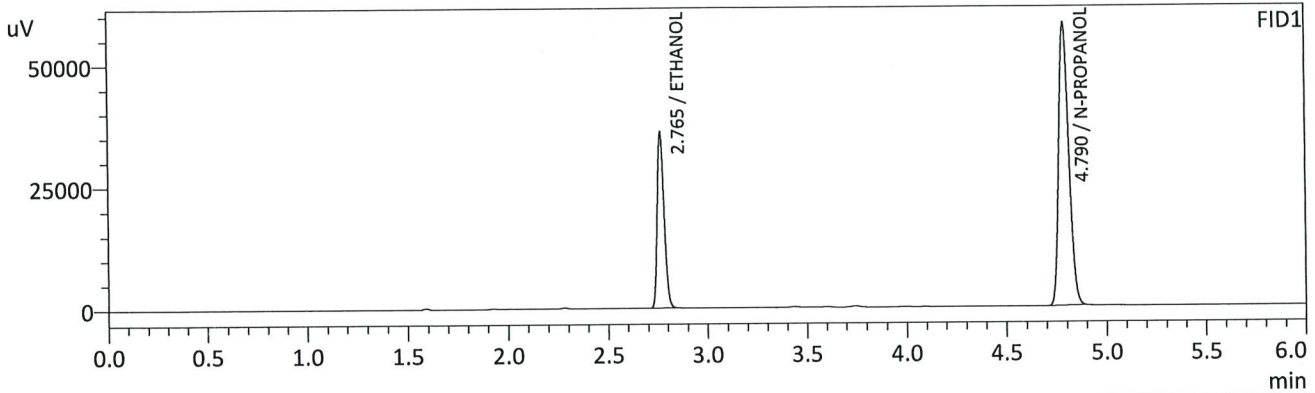

FID1



Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	0.2105	g/100cc	87005	35983
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	205047	57929
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	0.2106	g/100cc	85540	40993
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	200929	75044
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

15

Sample Name : QC2-2-B
 Vial # : 49
 Data Filename : QC2-2-B_1082025_049.gcd
 Method Filename : ALCOHOL_100725_TS.gcm
 Batch Filename : BATCH_100825_TS.gcb
 Date Acquired : 10/8/2025 6:31:14 PM
 Date Processed : 10/9/2025 7:57:04 AM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

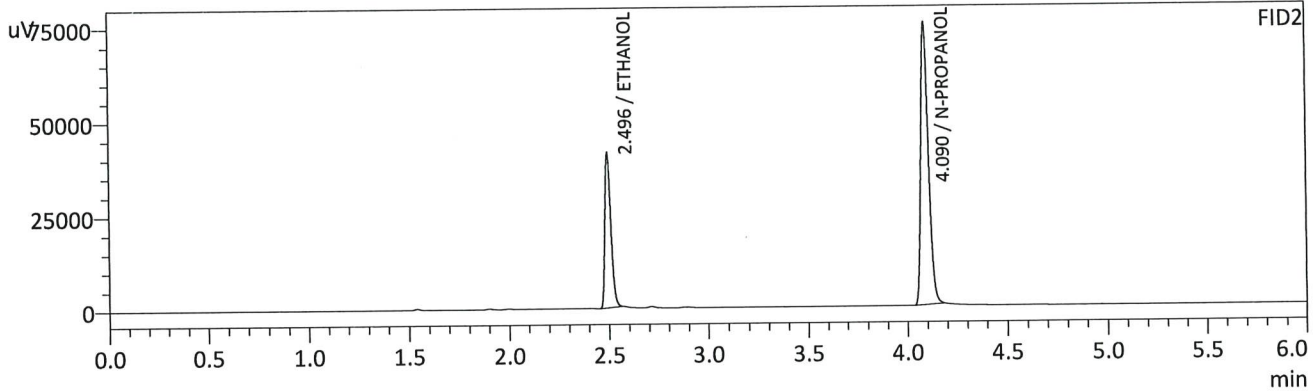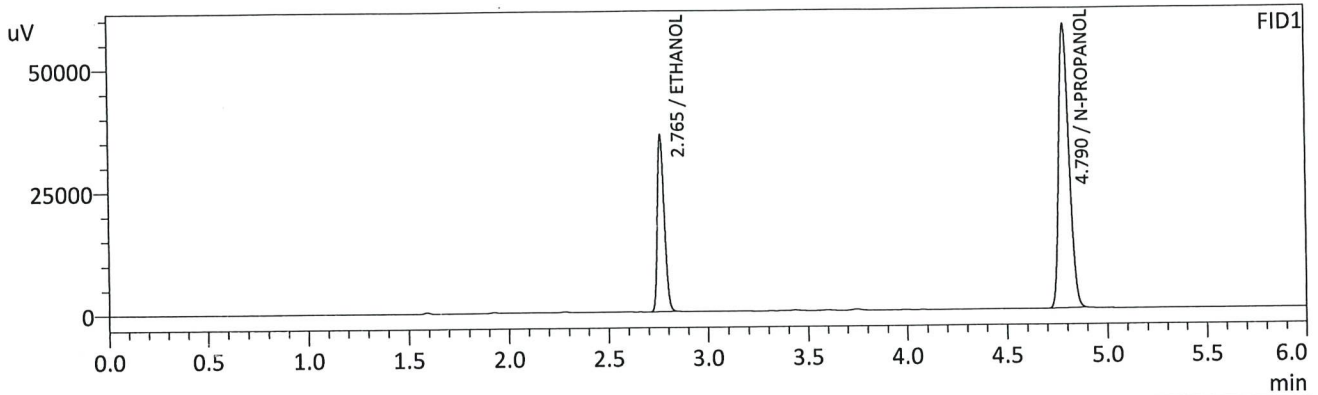

FID1



Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	0.2101	g/100cc	86904	35943
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	205253	57907
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	0.2099	g/100cc	85340	41000
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	201159	75163
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

15

Sample Name : INT STD BLK 3
 Vial # : 50
 Data Filename : INT STD BLK 3_1082025_050.gcd
 Method Filename : ALCOHOL_100725_TS.gcm
 Batch Filename : BATCH_100825_TS.gcb
 Date Acquired : 10/8/2025 6:40:38 PM
 Date Processed : 10/8/2025 6:46:40 PM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

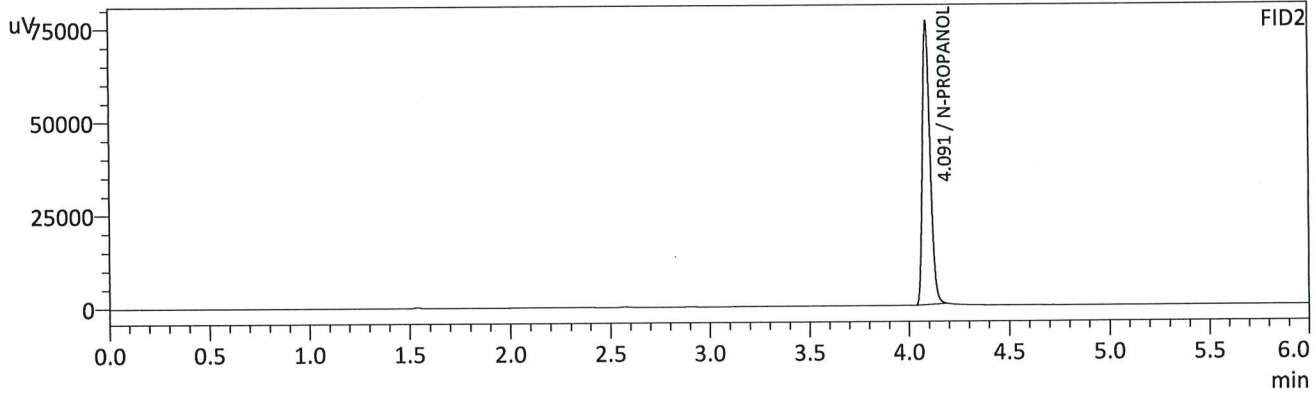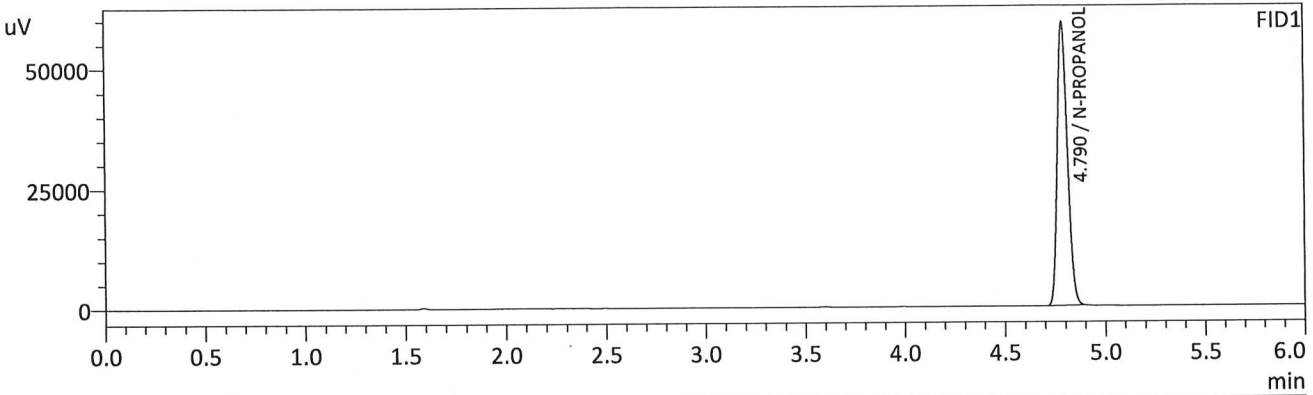

FID1

Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	208467	59020
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	203948	76104
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

TS

Region 5 Pocatello Blood Alcohol Analysis Batch Table

Shimadzu Nexis GC-2030 Serial Number: C12255850662

Shimadzu HS-20 Serial Number: C12595700014

LabSolutions Version 6.117

Copyright (C) 2008-2022 Shimadzu Corporation. All rights reserved.

Vial#	Sample Name	Sample Type	Method File	Data File	Level#
1	INT STD BLK 1	0:Unknown	ALCOHOL_100725_TS.gcm	1-5260 - INT STD BLK 1_9192025_001.gcd	0
2	MULTI-COMP MIX	0:Unknown	ALCOHOL_100725_TS.gcm	261 - MULTI-COMP MIX_9192025_002.gcd	1
3	INT STD BLK 2	0:Unknown	ALCOHOL_100725_TS.gcm	1-5262 - INT STD BLK 2_9192025_003.gcd	0
4	QC1-1	0:Unknown	ALCOHOL_100725_TS.gcm	1-5263 - QC1-1_9192025_004.gcd	0
5	QC1-1-B	0:Unknown	ALCOHOL_100725_TS.gcm	1-5264 - QC1-1-B_9192025_005.gcd	0
6	0.08 QA	0:Unknown	ALCOHOL_100725_TS.gcm	1-5265 - 0.08 QA_9192025_006.gcd	0
7	0.08 QA - B	0:Unknown	ALCOHOL_100725_TS.gcm	1-5266 - 0.08 QA - B_9192025_007.gcd	0
8	P2025-3039-1	0:Unknown	ALCOHOL_100725_TS.gcm	1-5267 - M2025-3540-1_9192025_008.gcd	0
9	P2025-3039-1-B	0:Unknown	ALCOHOL_100725_TS.gcm	-5268 - M2025-3540-1-B_9192025_009.gcd	0
10	P2025-3040-1	0:Unknown	ALCOHOL_100725_TS.gcm	1-5269 - P2025-2833-1_9192025_010.gcd	0
11	P2025-3040-1-B	0:Unknown	ALCOHOL_100725_TS.gcm	-5270 - P2025-2833-1-B_9192025_011.gcd	0
12	P2025-3041-1	0:Unknown	ALCOHOL_100725_TS.gcm	1-5271 - P2025-2856-1_9192025_012.gcd	0
13	P2025-3041-1-B	0:Unknown	ALCOHOL_100725_TS.gcm	-5272 - P2025-2856-1-B_9192025_013.gcd	0
14	P2025-3042-1	0:Unknown	ALCOHOL_100725_TS.gcm	1-5273 - P2025-2858-1_9192025_014.gcd	0
15	P2025-3042-1-B	0:Unknown	ALCOHOL_100725_TS.gcm	-5274 - P2025-2858-1-B_9192025_015.gcd	0
16	P2025-3044-1	0:Unknown	ALCOHOL_100725_TS.gcm	1-5275 - P2025-2862-1_9192025_016.gcd	0
17	P2025-3044-1-B	0:Unknown	ALCOHOL_100725_TS.gcm	-5276 - P2025-2862-1-B_9192025_017.gcd	0
18	P2025-3045-1	0:Unknown	ALCOHOL_100725_TS.gcm	1-5277 - P2025-2863-1_9192025_018.gcd	0
19	P2025-3045-1-B	0:Unknown	ALCOHOL_100725_TS.gcm	-5278 - P2025-2863-1-B_9192025_019.gcd	0
20	P2025-3054-1	0:Unknown	ALCOHOL_100725_TS.gcm	1-5279 - P2025-2864-1_9192025_020.gcd	0
21	P2025-3054-1-B	0:Unknown	ALCOHOL_100725_TS.gcm	-5280 - P2025-2864-1-B_9192025_021.gcd	0
22	P2025-3064-1	0:Unknown	ALCOHOL_100725_TS.gcm	1-5281 - P2025-2865-1_9192025_022.gcd	0
23	P2025-3064-1-B	0:Unknown	ALCOHOL_100725_TS.gcm	-5282 - P2025-2865-1-B_9192025_023.gcd	0
24	P2025-3072-1	0:Unknown	ALCOHOL_100725_TS.gcm	1-5283 - P2025-2876-1_9192025_024.gcd	0
25	P2025-3072-1-B	0:Unknown	ALCOHOL_100725_TS.gcm	-5284 - P2025-2876-1-B_9192025_025.gcd	0
26	QC2-1	0:Unknown	ALCOHOL_100725_TS.gcm	1-5285 - QC2-1_9192025_026.gcd	0
27	QC2-1-B	0:Unknown	ALCOHOL_100725_TS.gcm	1-5286 - QC2-1-B_9192025_027.gcd	0
28	P2025-3074-1	0:Unknown	ALCOHOL_100725_TS.gcm	1-5287 - P2025-2881-1_9192025_028.gcd	0
29	P2025-3074-1-B	0:Unknown	ALCOHOL_100725_TS.gcm	-5288 - P2025-2881-1-B_9192025_029.gcd	0
30	P2025-3075-1	0:Unknown	ALCOHOL_100725_TS.gcm	1-5289 - P2025-2896-1_9192025_030.gcd	0
31	P2025-3075-1-B	0:Unknown	ALCOHOL_100725_TS.gcm	-5290 - P2025-2896-1-B_9192025_031.gcd	0
32	P2025-3076-1	0:Unknown	ALCOHOL_100725_TS.gcm	1-5291 - P2025-2901-1_9192025_032.gcd	0
33	P2025-3076-1-B	0:Unknown	ALCOHOL_100725_TS.gcm	-5292 - P2025-2901-1-B_9192025_033.gcd	0
34	P2025-3078-1	0:Unknown	ALCOHOL_100725_TS.gcm	1-5293 - P2025-2904-1_9192025_034.gcd	0
35	P2025-3078-1-B	0:Unknown	ALCOHOL_100725_TS.gcm	-5294 - P2025-2904-1-B_9192025_035.gcd	0
36	P2025-3079-1	0:Unknown	ALCOHOL_100725_TS.gcm	1-5295 - P2025-2921-3_9192025_036.gcd	0
37	P2025-3079-1-B	0:Unknown	ALCOHOL_100725_TS.gcm	-5296 - P2025-2921-3-B_9192025_037.gcd	0
38	P2025-3082-1	0:Unknown	ALCOHOL_100725_TS.gcm	1-5297 - P2025-2935-1_9192025_038.gcd	0
39	P2025-3082-1-B	0:Unknown	ALCOHOL_100725_TS.gcm	-5298 - P2025-2935-1-B_9192025_039.gcd	0
40	P2025-3083-1	0:Unknown	ALCOHOL_100725_TS.gcm	1-5299 - P2025-2936-1_9192025_040.gcd	0
41	P2025-3083-1-B	0:Unknown	ALCOHOL_100725_TS.gcm	-5300 - P2025-2936-1-B_9192025_041.gcd	0
42	P2025-3086-1	0:Unknown	ALCOHOL_100725_TS.gcm	1-5301 - P2025-2937-1_9192025_042.gcd	0
43	P2025-3086-1-B	0:Unknown	ALCOHOL_100725_TS.gcm	-5302 - P2025-2937-1-B_9192025_043.gcd	0
44	P2025-3087-1	0:Unknown	ALCOHOL_100725_TS.gcm	1-5303 - P2025-2938-1_9192025_044.gcd	0
45	P2025-3087-1-B	0:Unknown	ALCOHOL_100725_TS.gcm	-5304 - P2025-2938-1-B_9192025_045.gcd	0
46	P2025-3089-1	0:Unknown	ALCOHOL_100725_TS.gcm		0
47	P2025-3089-1-B	0:Unknown	ALCOHOL_100725_TS.gcm		0
48	QC2-2	0:Unknown	ALCOHOL_100725_TS.gcm	1-5305 - QC2-2_9192025_046.gcd	0
49	QC2-2-B	0:Unknown	ALCOHOL_100725_TS.gcm	1-5306 - QC2-2-B_9192025_047.gcd	0
50	INT STD BLK 3	0:Unknown	ALCOHOL_100725_TS.gcm	1-5307 - INT STD BLK 3_9192025_048.gcd	0

Region 5 Pocatello Blood Alcohol Analysis Batch Table

Shimadzu Nexis GC-2030 Serial Number: C12255850662

Shimadzu HS-20 Serial Number: C12595700014



LabSolutions Version 6.117

Copyright (C) 2008-2022 Shimadzu Corporation. All rights reserved.

Vial#	Sample Name	Sample Type	Method File	Data File	Level#
50	INT STD BLK	0:Unknown	ALCOHOL_100725_TS.gcm	1-5415 - INT STD BLK_1092025_001.gcd	0
51	DFE	0:Unknown	ALCOHOL_100725_TS.gcm	1-5416 - DFE_1092025_002.gcd	1
52	INT STD BLK 2	0:Unknown	ALCOHOL_100725_TS.gcm	1-5417 - INT STD BLK 2_1092025_003.gcd	0

15

Sample Name : INT STD BLK
 Vial # : 50
 Data Filename : INT STD BLK_1092025_001.gcd
 Method Filename : ALCOHOL_100725_TS.gcm
 Batch Filename : DFE_100925_TS.gcb
 Date Acquired : 10/9/2025 8:42:44 AM
 Date Processed : 10/9/2025 8:48:46 AM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

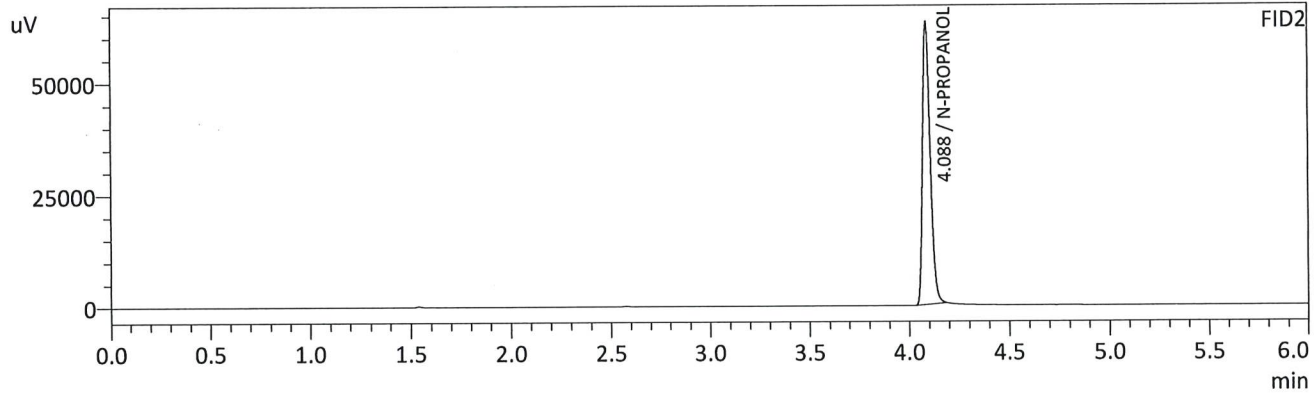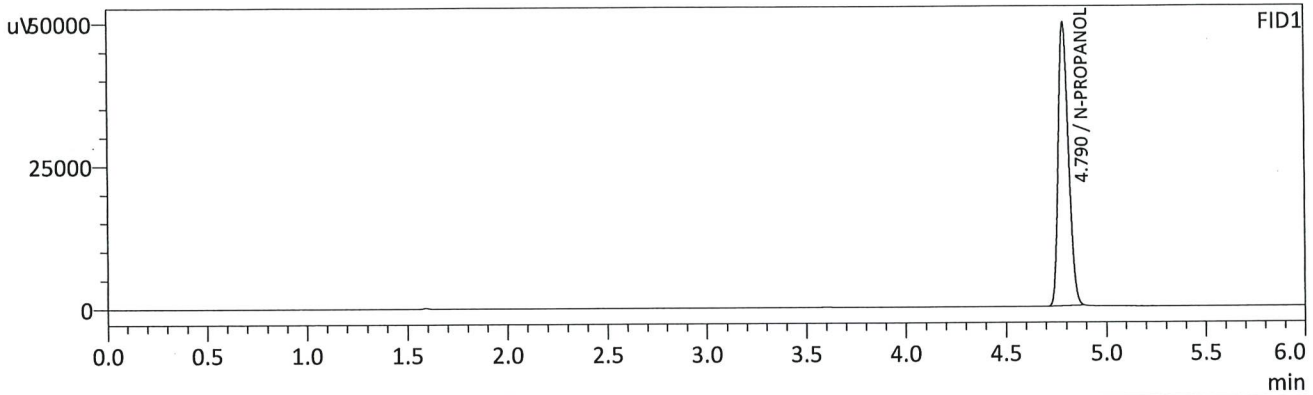

FID1



Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	174614	49641
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	168372	62655
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

TS

Sample Name : DFE
 Vial # : 51
 Data Filename : DFE_1092025_002.gcd
 Method Filename : ALCOHOL_100725_TS.gcm
 Batch Filename : DFE_100925_TS.gcb
 Date Acquired : 10/9/2025 8:52:14 AM
 Date Processed : 10/9/2025 8:58:14 AM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

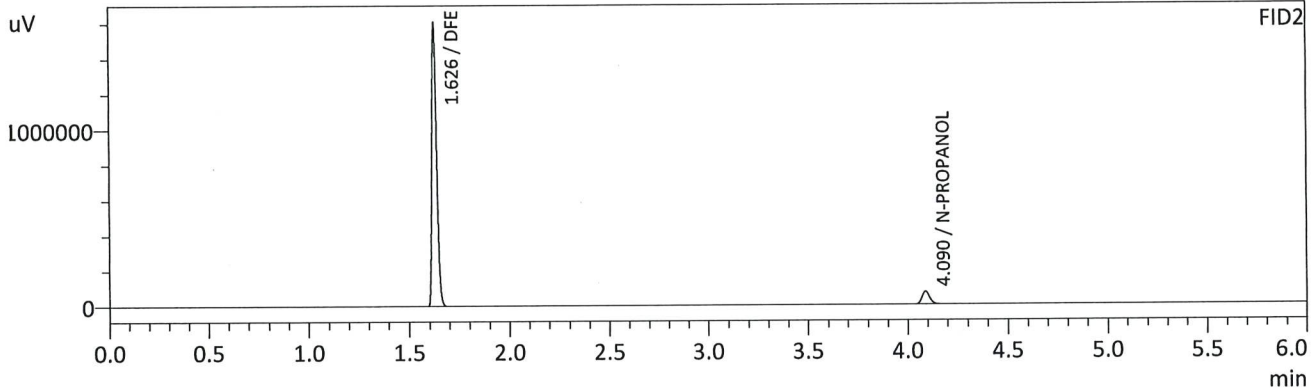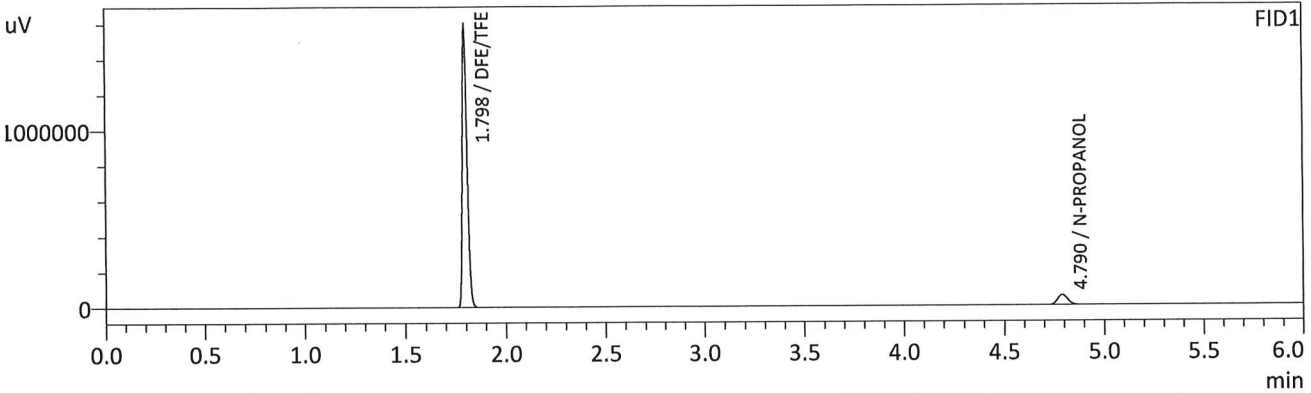

FID1



Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	200451	57256
DFE/TFE	0.0000	g/100cc	2660402	1570545
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	193819	72907
DFE	0.0000	g/100cc	2638989	1598252
TFE	--	g/100cc	--	--

15

Sample Name : INT STD BLK 2
 Vial # : 52
 Data Filename : INT STD BLK 2_1092025_003.gcd
 Method Filename : ALCOHOL_100725_TS.gcm
 Batch Filename : DFE_100925_TS.gcb
 Date Acquired : 10/9/2025 9:01:34 AM
 Date Processed : 10/9/2025 9:07:37 AM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

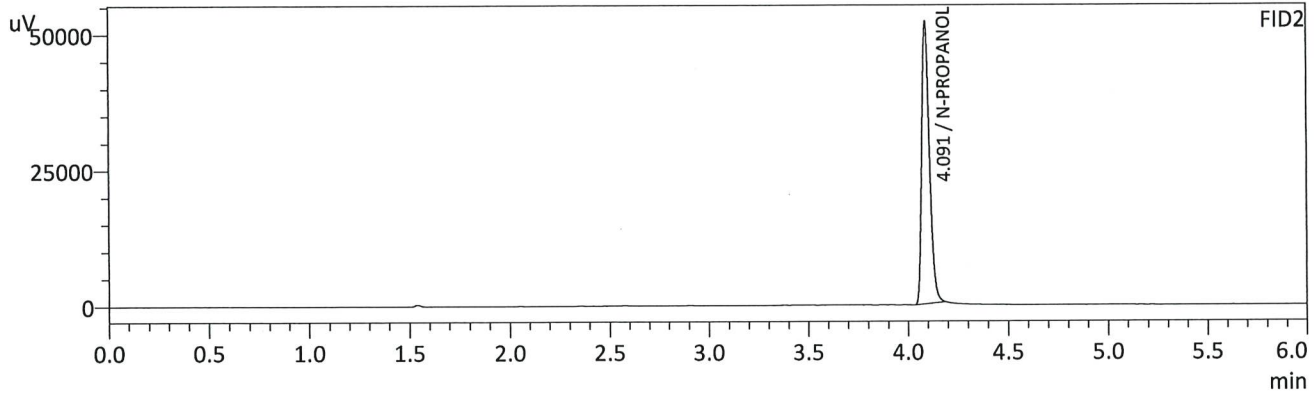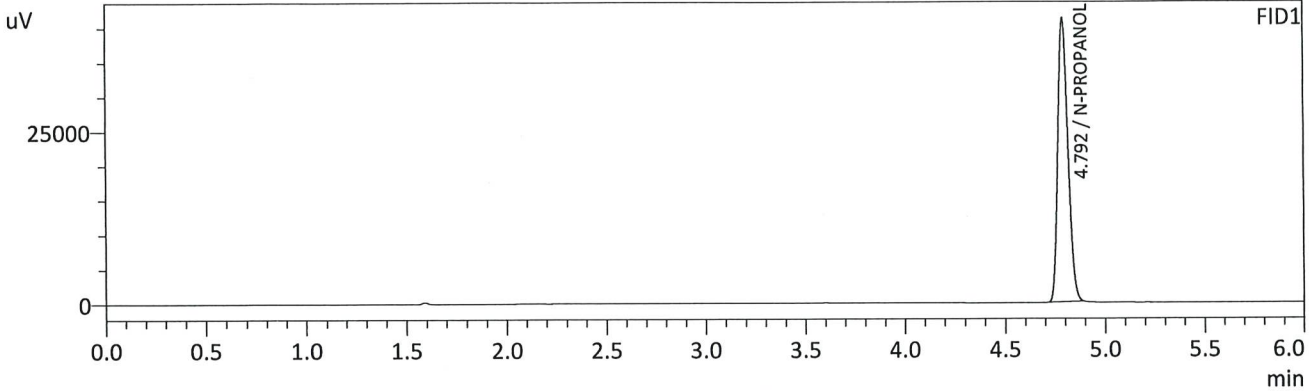

FID1

Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	145461	41070
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	140227	51939
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

B