

---

## WORK INSTRUCTIONS

---

### 2.4.2 Confirmation for Gamma Hydroxybutyrate (GHB) in Urine utilizing Toxi-B Extraction Tubes

---

#### REFERENCE MATERIAL

---

##### GHB Positive Control

- Stock Solutions  
1 mg/mL single component Gamma Hydroxybutyric Acid (GHB) reference solution.
- Direct spiking  
Two positive controls:  
Spike one sample containing 4050uL negative urine with 450uL of GHB 1mg/mL.  
Spike one sample containing 3600uL negative urine with 900uL of GHB 1mg/mL.

##### Non-extracted GHB Reference Material

- Stock Solution  
1 mg/mL GHB
  - Direct spiking  
Spike tapered bottom tube with 10uL, dry and derivatize.
-

## WORK INSTRUCTIONS

### 2.4.2 Confirmation for Gamma Hydroxybutyrate (GHB) in Urine utilizing Toxi-B Extraction Tubes

#### Toxi-B Tube Extraction


Reagents

**TOXI-TUBES B**

Qualitative Controls

**Spiked Positive controls**

**Negative Urine**

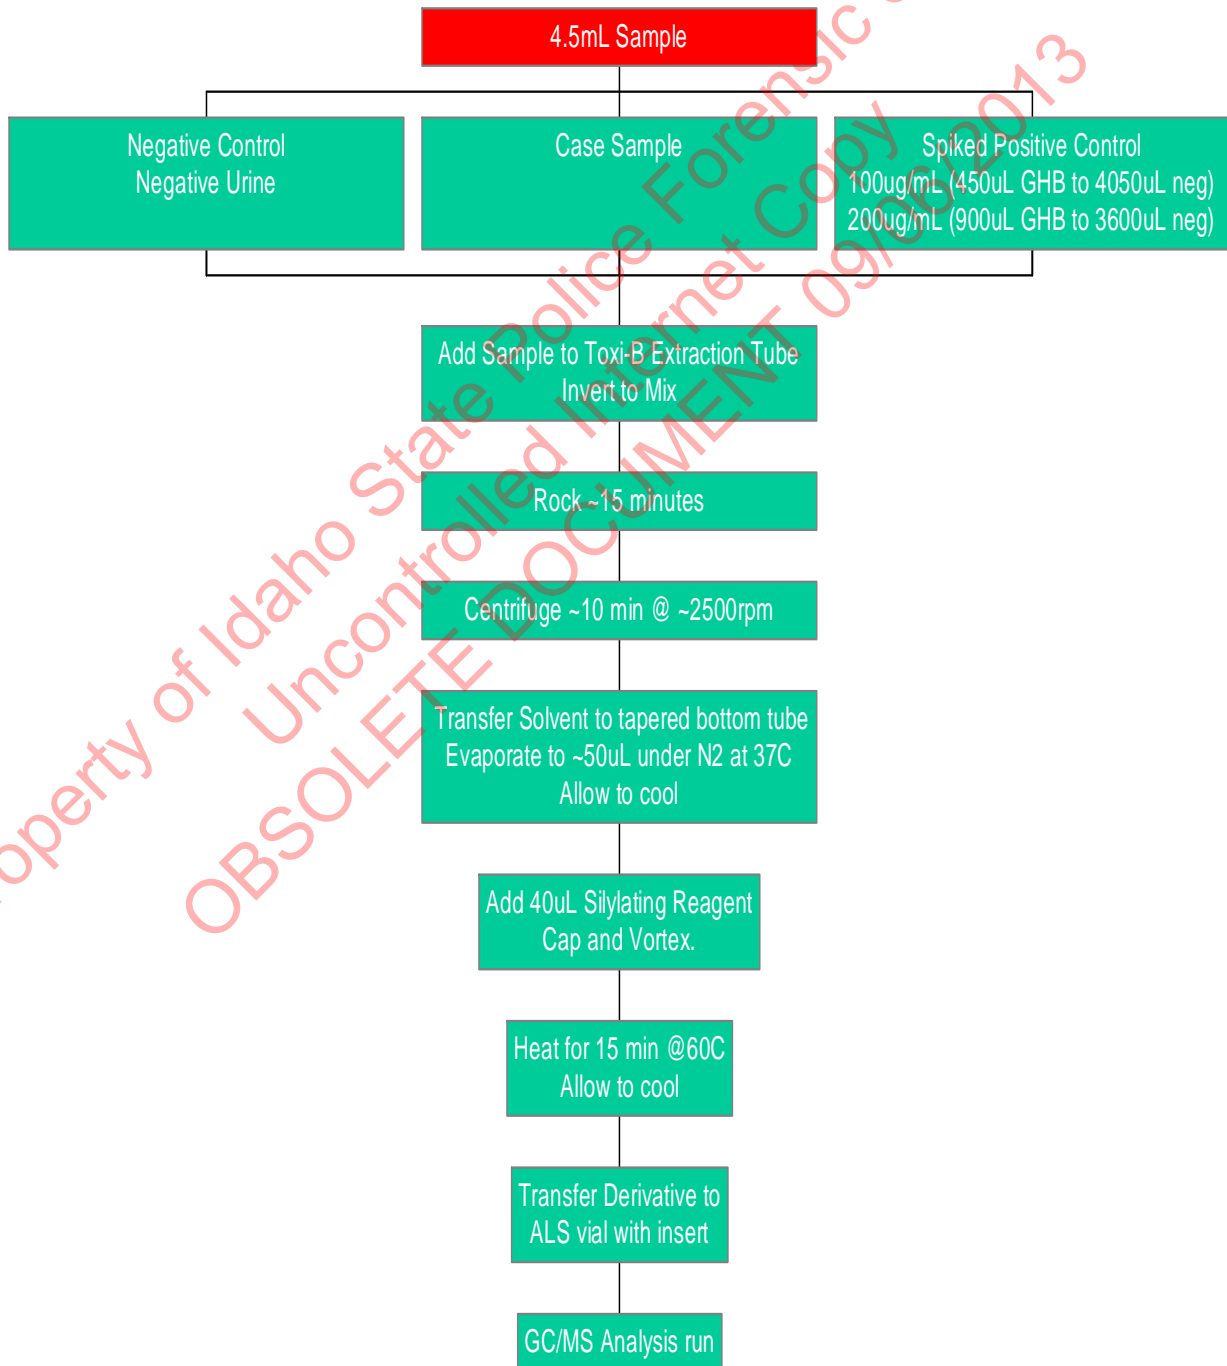

## WORK INSTRUCTIONS

### 2.4.2 Confirmation for Gamma Hydroxybutyrate (GHB) in Urine utilizing Toxi-B Extraction Tubes

#### *Revision History*

Revision No.	Issue Date	Revision/Comments
0	9/27/2012	Original Issue

Property of Idaho State Police Forensic Services  
Uncontrolled Internet Copy  
OBSOLETE DOCUMENT 09/06/2013