

Quantitative Analysis for Ethanol & Qualitative Analysis for Other Volatiles

Analytical Method(s): 1.0

Device: Hamilton MICROLAB 5034 Liquid Processor/Dilutor Serial Number: MD-96BC1382/MD944M10010

Volatiles Quality Assurance Controls

Run Date(s): 07/13/2017-07/14/2017

Calibration Date: 7/7/2017

Control level	Expiration	Lot #	Target Value	Acceptable Range	Overall Results	
					Column 1	Column 2
Level 1	Jul-18	1407031	0.0780	0.0702 - 0.0858	0.0788	g/100cc
					0.0813	g/100cc
						g/100cc
Level 2	Jul-18	1407032	0.2020	0.1818 - 0.2222	0.1994	g/100cc
					0.2086	g/100cc
Multi-Component Mixture		Exp: Oct 2019	Lot #	FN09231404	OK	
Curve Fit:		Column 1	0.99999	Column 2	0.99992	

Ethanol Calibration Reference Material								
Calibrator level	Expiration	Ceriliant Lot #	Target Value	Acceptable Range	Column 1	Column 2	Precision	Mean
0.050	Jul-19	FN06231406	0.050	0.045 - 0.055	0.0508	0.0528	0.002	0.0518
0.080			0.080	0.072 - 0.088			0	#DIV/0!
0.100	Jun-20	FN06181501	0.100	0.090 - 0.110	0.0997	0.0995	0.0002	0.0996
0.200	Oct-20	FN07201502	0.200	0.180 - 0.220	0.1991	0.1976	0.0015	0.1983
0.300	Feb-21	FN02121601	0.300	0.270 - 0.330	0.3001	0.2984	0.0017	0.2992
0.400			0.400	0.360 - 0.440			0	#DIV/0!
0.500	Aug-19	FN07031402	0.500	0.450 - 0.550	0.5003	0.5018	0.0015	0.501

Aqueous Controls					
Control level	Expiration	Ceriliant Lot #	Target Value	Acceptable Range	Overall Results
0.080	Nov-20	FN10281510	0.08000	0.076 - 0.084	0.083 g/100cc

Issued: 4/22/2015


~Any information on this document can be changed for laboratory use, except for the precision and mean determination formulas.

Volatiles QA/QC data spreadsheet Rev 5

Issuing Authority: Quality Manager


JK

Worklist: 1810

<u>LAB CASE</u>	<u>ITEM</u>	<u>TASK ID</u>	<u>DESCRIPTION</u>	
M2017-3013	1	88893	Alcohol Analysis	
M2017-3059	1	89113	Alcohol Analysis	
M2017-3060	1	89223	Alcohol Analysis	
M2017-3061	1	89237	Alcohol Analysis	
M2017-3063	1	89242	Alcohol Analysis	
M2017-3066	1	89299	Alcohol Analysis	
M2017-3072	1	89338	Alcohol Analysis	
M2017-3082	1	89365	Alcohol Analysis	
M2017-3089	1	89379	Alcohol Analysis	
M2017-3090	1	89383	Alcohol Analysis	
M2017-3091	1	89391	Alcohol Analysis	
M2017-3092	1	89395	Alcohol Analysis	
M2017-3103	1	89463	Alcohol Analysis	
M2017-3112	1	89492	Alcohol Analysis	
M2017-3113	1	89493	Alcohol Analysis	
M2017-3151	1	89596	Alcohol Analysis	
M2017-3152	1	89600	Alcohol Analysis	
M2017-3153	1	89604	Alcohol Analysis	
M2017-3157	3	89949	Alcohol Analysis	
M2017-3158	1	89664	Alcohol Analysis	
M2017-3159	1	89666	Alcohol Analysis	
M2017-3160	1	89667	Alcohol Analysis	
M2017-3161	1	89668	Alcohol Analysis	


Worklist: 1810

<u>LAB CASE</u>	<u>ITEM</u>	<u>TASK ID</u>	<u>DESCRIPTION</u>
M2017-3162	1	89670	Alcohol Analysis
M2017-3182	1	89696	Alcohol Analysis
M2017-3194	1	89722	Alcohol Analysis
M2017-3195	1	89723	Alcohol Analysis
P2017-1380	2	89229	Alcohol Analysis
P2017-1428	2	89387	Alcohol Analysis

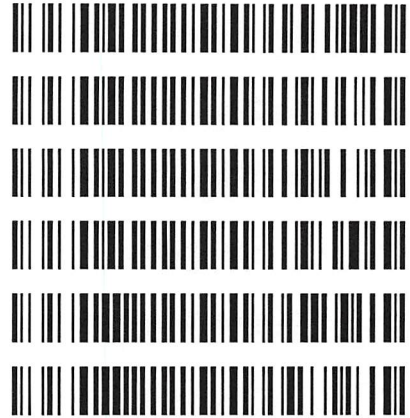

ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STD BLK 1
 Laboratory : Meridian
 Injection Date : Jul 13, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

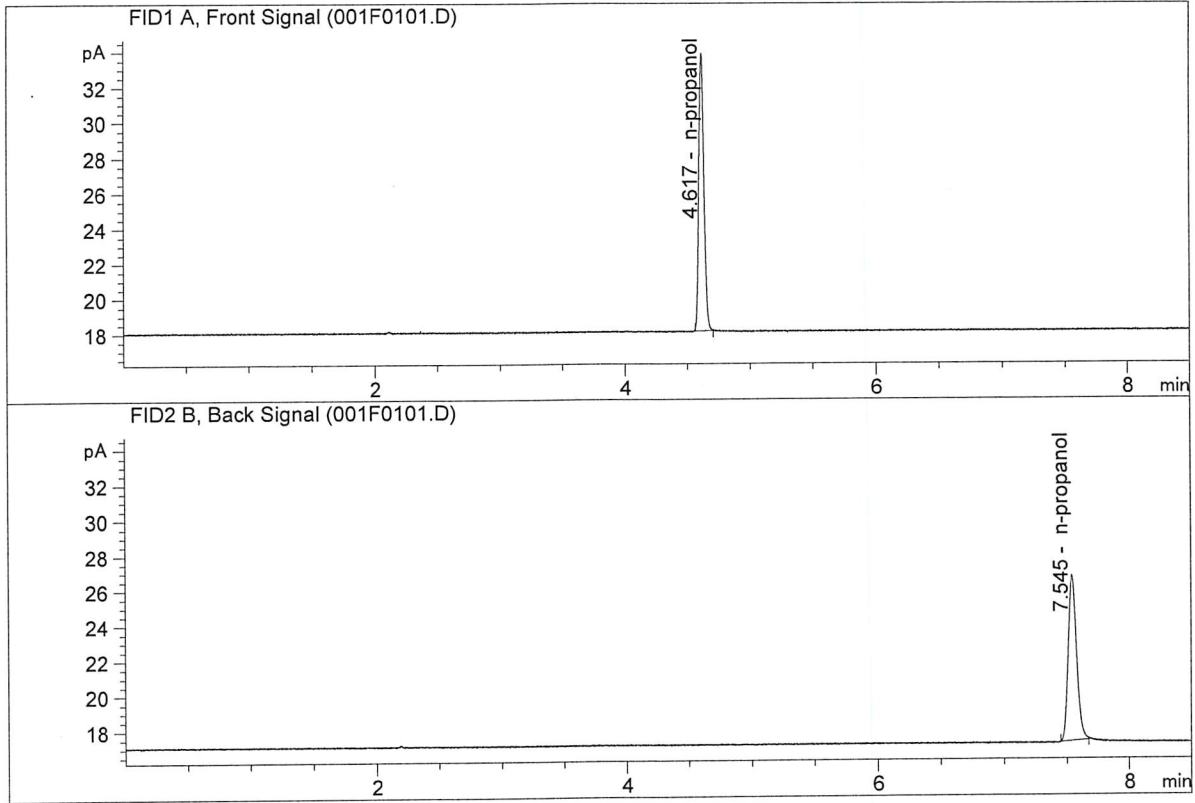


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	44.90694	1.0000	g/100cc
4.	n-Propanol	Column 2:	45.57406	1.0000	g/100cc

JG

ISP Forensic Services Blood Alcohol Report

Sample Name : MIX VOL FN09231404
 Laboratory : Meridian
 Injection Date : Jul 13, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

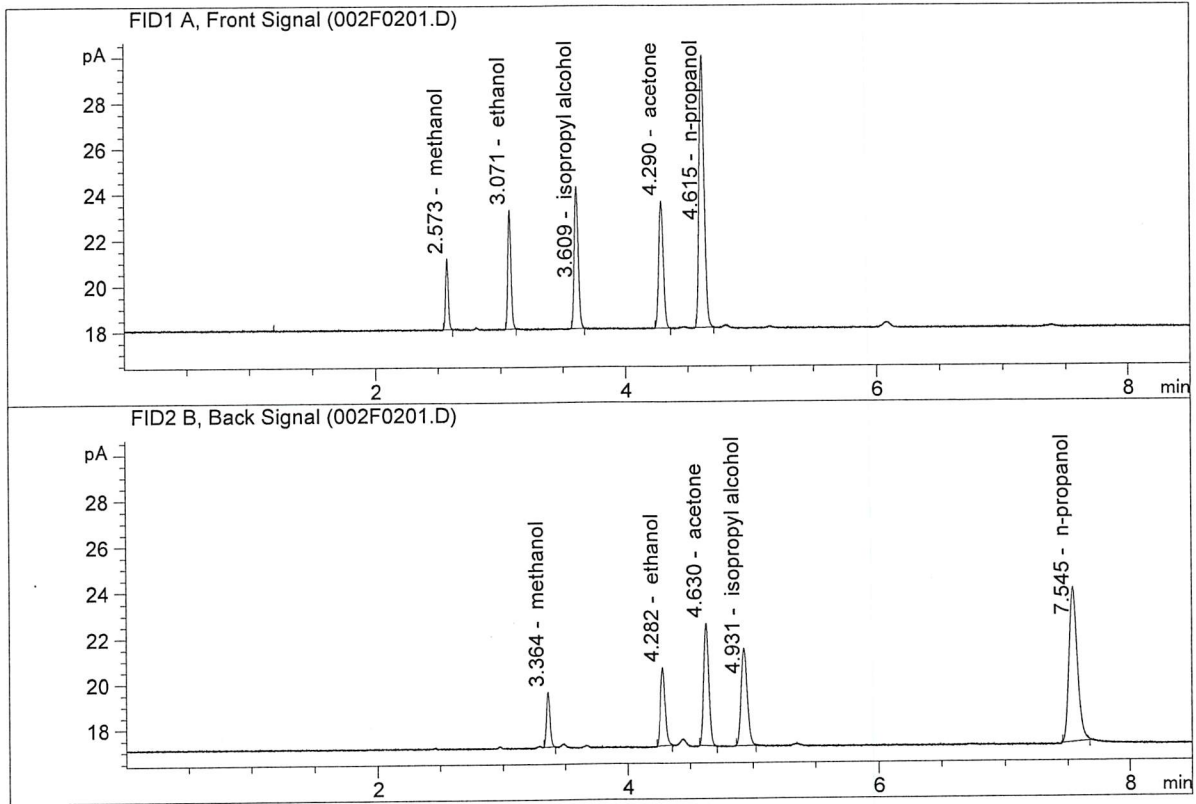

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	9.20003	0.1402	g/100cc
2.	Ethanol	Column 2:	9.19377	0.1402	g/100cc
3.	n-Propanol	Column 1:	33.41555	1.0000	g/100cc
4.	n-Propanol	Column 2:	32.97975	1.0000	g/100cc

JG

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC1-1

Analysis Date(s): 13 Jul 2017

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.0780	0.0787	0.0007	0.0783	0.0788	
(g/100cc)	0.0784	0.0803	0.0019	0.0793		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: ALCOHOL.M
Hamilton Auto-Dilutor Serial Number:
MD96BC1382/MD94AM10010

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.078	0.074	0.082	0.004

	Reported Result	
	0.078	

Calibration and control data are stored centrally.

Issued: 12/30/2016


Volatiles BAC Calculation Spreadsheet Rev 4

Issuing Authority: Quality Manager

JG

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-1-A
 Laboratory : Meridian
 Injection Date : Jul 13, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

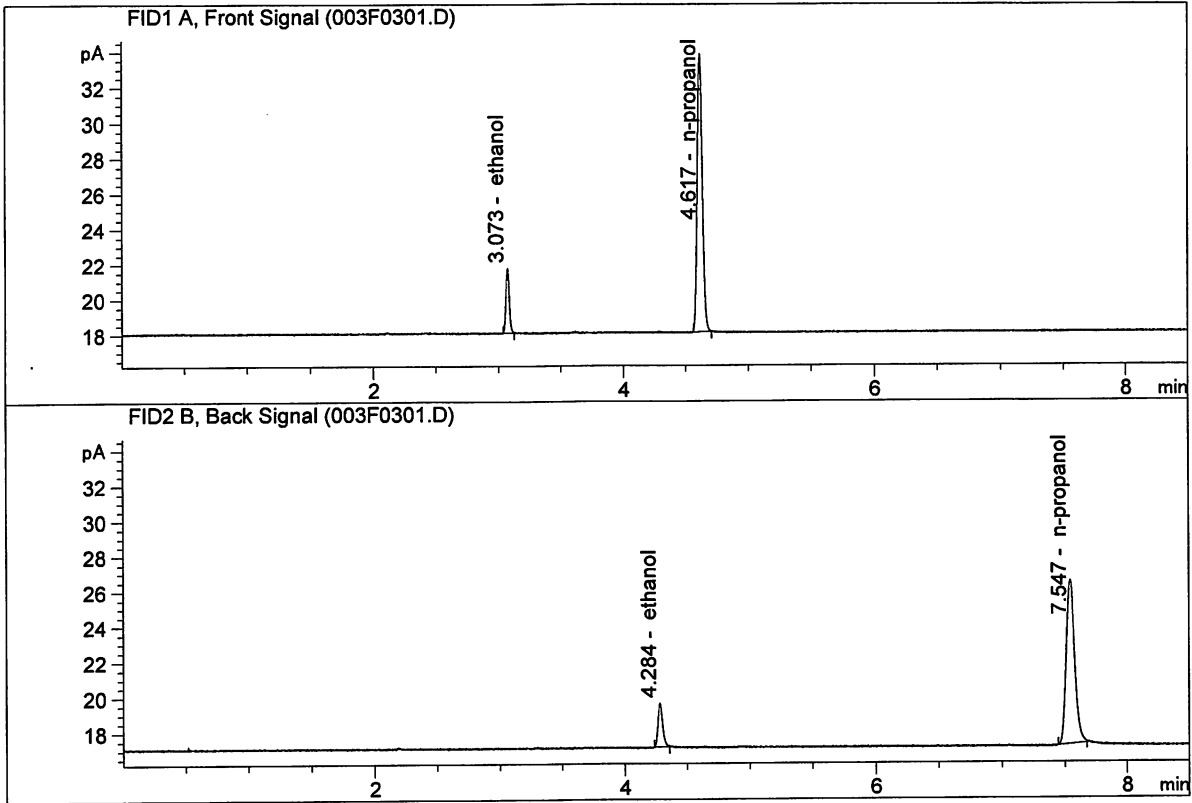


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	6.79206	0.0780	g/100cc
2.	Ethanol	Column 2:	6.73999	0.0787	g/100cc
3.	n-Propanol	Column 1:	44.73539	1.0000	g/100cc
4.	n-Propanol	Column 2:	44.83661	1.0000	g/100cc

JG

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-1-B
 Laboratory : Meridian
 Injection Date : Jul 13, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

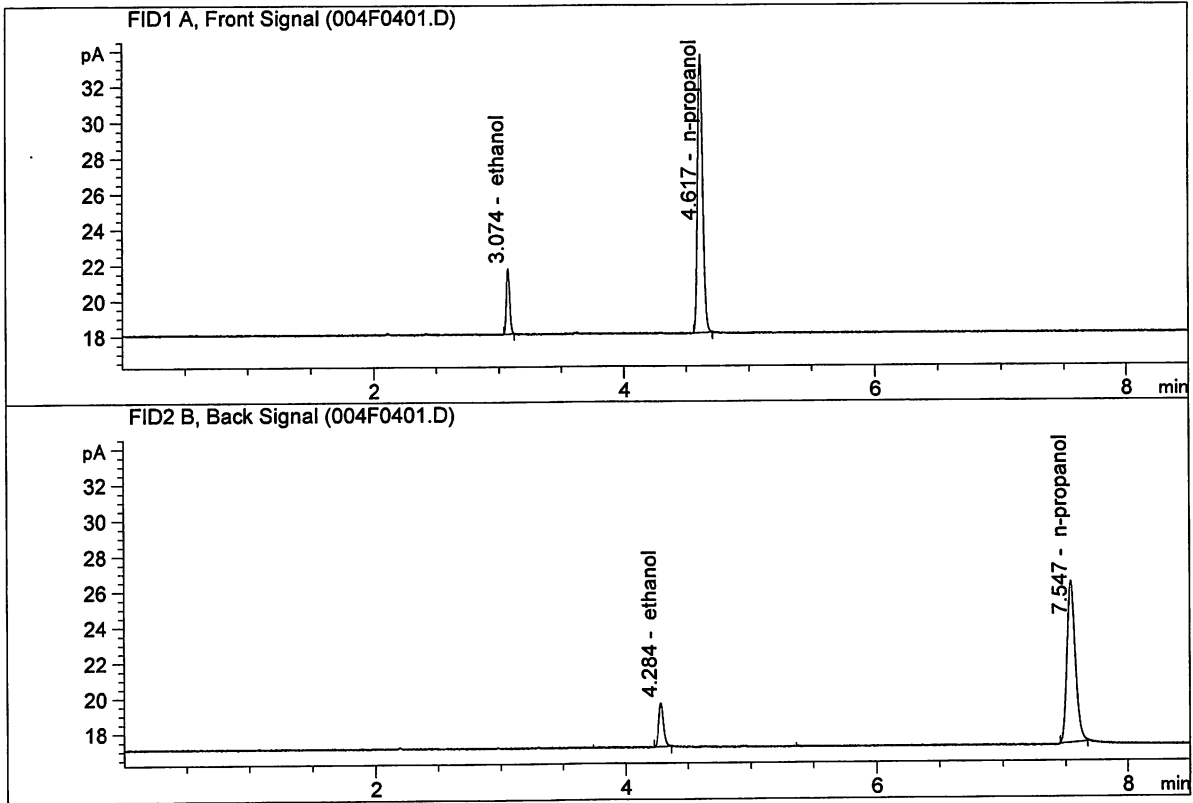

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	6.76312	0.0784	g/100cc
2.	Ethanol	Column 2:	6.79546	0.0803	g/100cc
3.	n-Propanol	Column 1:	44.36201	1.0000	g/100cc
4.	n-Propanol	Column 2:	44.17336	1.0000	g/100cc

JG

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: 0.08 FN10281510

Analysis Date(s): 13 Jul 2017

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.0804	0.0819	0.0015	0.0811	0.0830	
(g/100cc)	0.0842	0.0857	0.0015	0.0849		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: ALCOHOL.M
Hamilton Auto-Dilutor Serial Number:
MD96BC1382/MD94AM10010

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.083	0.078	0.088	0.005

Reported Result	
0.083	

Calibration and control data are stored centrally.

Issued: 12/30/2016


Volatiles BAC Calculation Spreadsheet Rev 4

Issuing Authority: Quality Manager

JG

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.08 FN10281510-A
 Laboratory : Meridian
 Injection Date : Jul 13, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

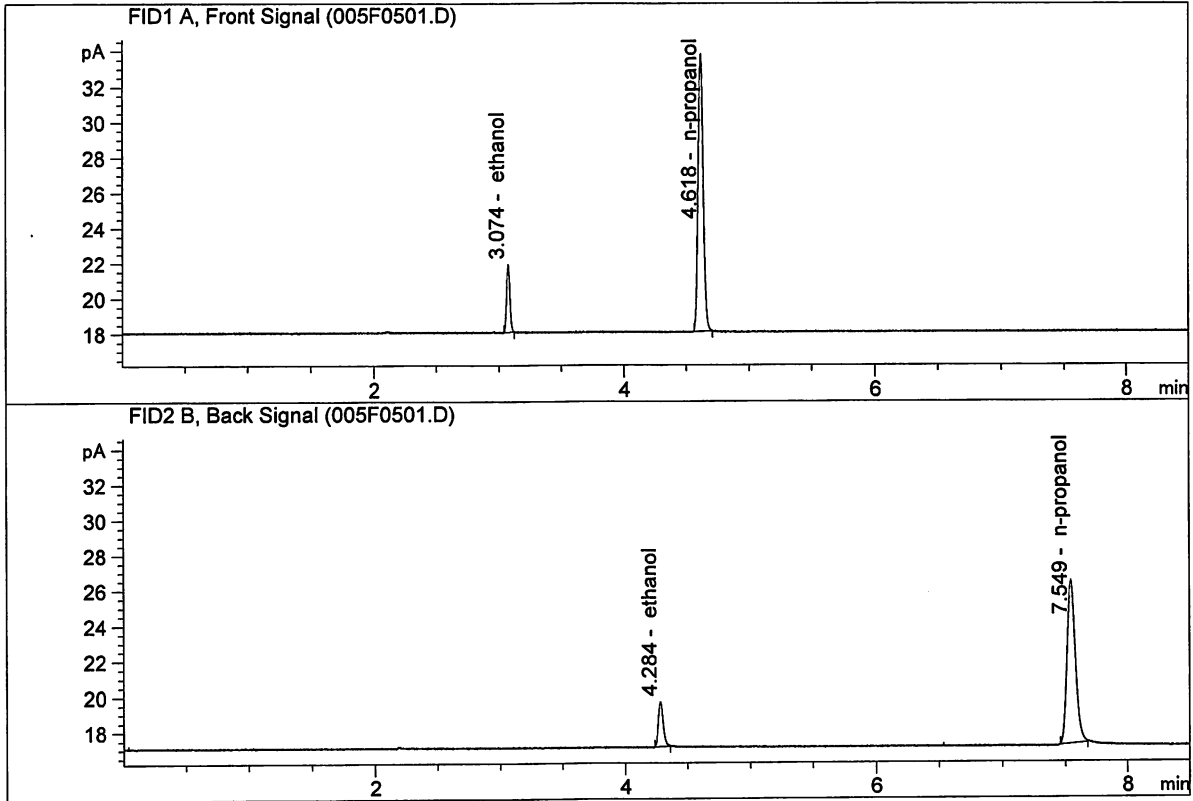


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.00339	0.0804	g/100cc
2.	Ethanol	Column 2:	6.99130	0.0819	g/100cc
3.	n-Propanol	Column 1:	44.73703	1.0000	g/100cc
4.	n-Propanol	Column 2:	44.53451	1.0000	g/100cc

JG

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.08 FN10281510-B
 Laboratory : Meridian
 Injection Date : Jul 13, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

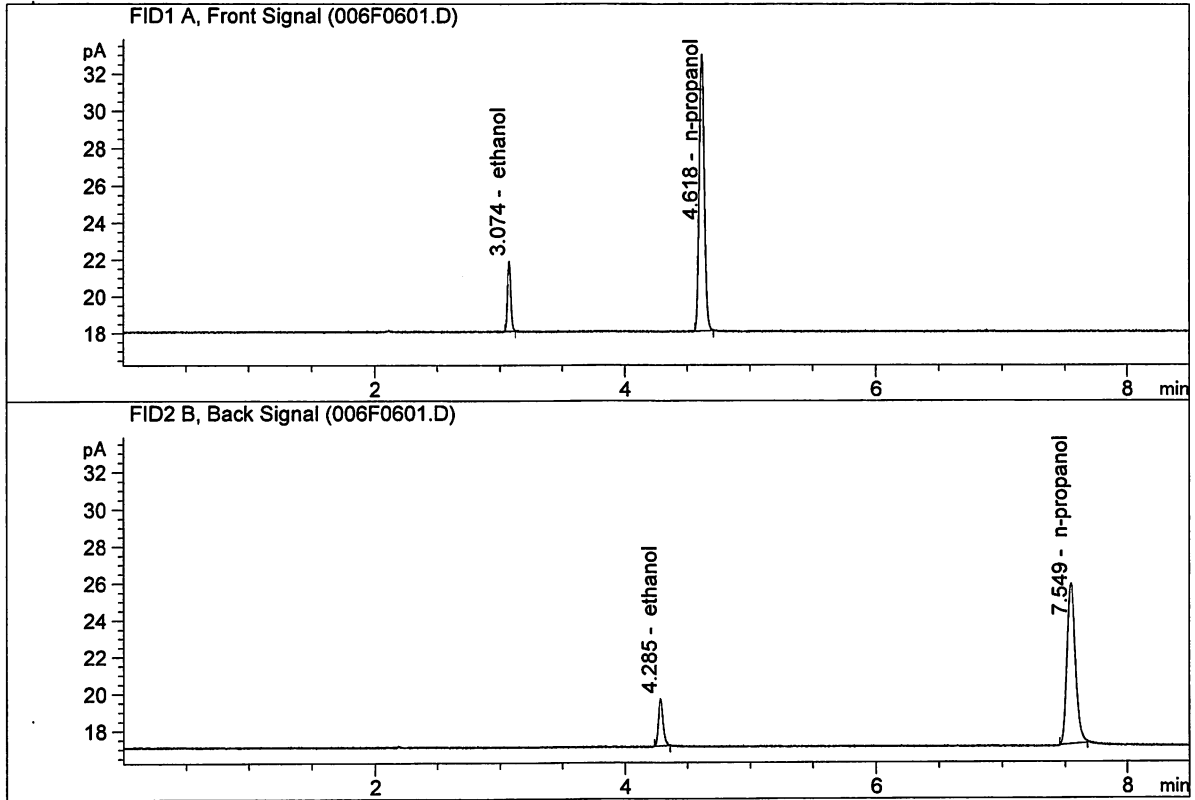

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	6.96958	0.0842	g/100cc
2.	Ethanol	Column 2:	6.95226	0.0857	g/100cc
3.	n-Propanol	Column 1:	42.50531	1.0000	g/100cc
4.	n-Propanol	Column 2:	42.15434	1.0000	g/100cc

JG

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC2-1

Analysis Date(s): 13 Jul 2017

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.1998	0.1994	0.0004	0.1996	0.1994	
(g/100cc)	0.1993	0.1994	0.0001	0.1993		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: ALCOHOL.M
Hamilton Auto-Dilutor Serial Number:
MD96BC1382/MD94AM10010

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.199	0.189	0.209	0.010

	Reported Result	
	0.199	

Calibration and control data are stored centrally.

Issued: 12/30/2016


Volatiles BAC Calculation Spreadsheet Rev 4

Issuing Authority: Quality Manager

JG

ISP Forensic Services Blood Alcohol Report


Sample Name : QC2-1-A
 Laboratory : Meridian
 Injection Date : Jul 13, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

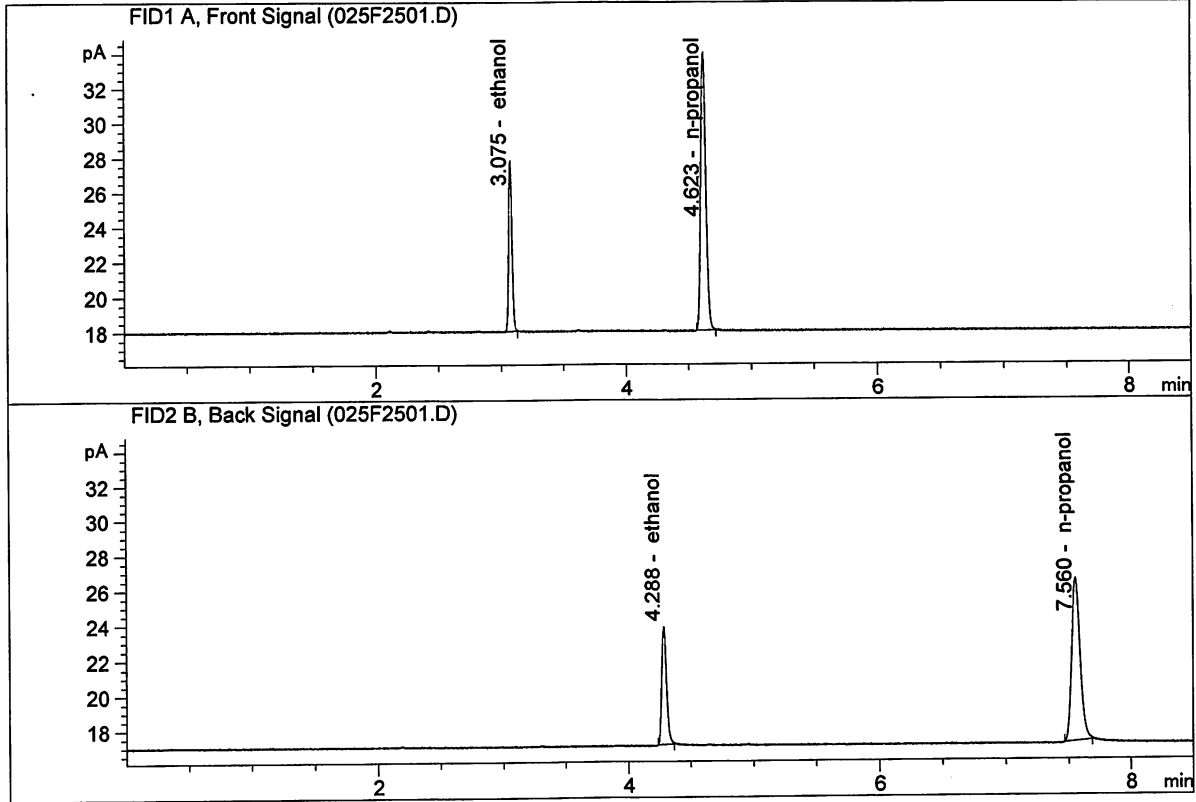

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	17.89491	0.1998	g/100cc
2.	Ethanol	Column 2:	18.11646	0.1994	g/100cc
3.	n-Propanol	Column 1:	45.47340	1.0000	g/100cc
4.	n-Propanol	Column 2:	45.01413	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report

Sample Name : QC2-1-B
 Laboratory : Meridian
 Injection Date : Jul 13, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

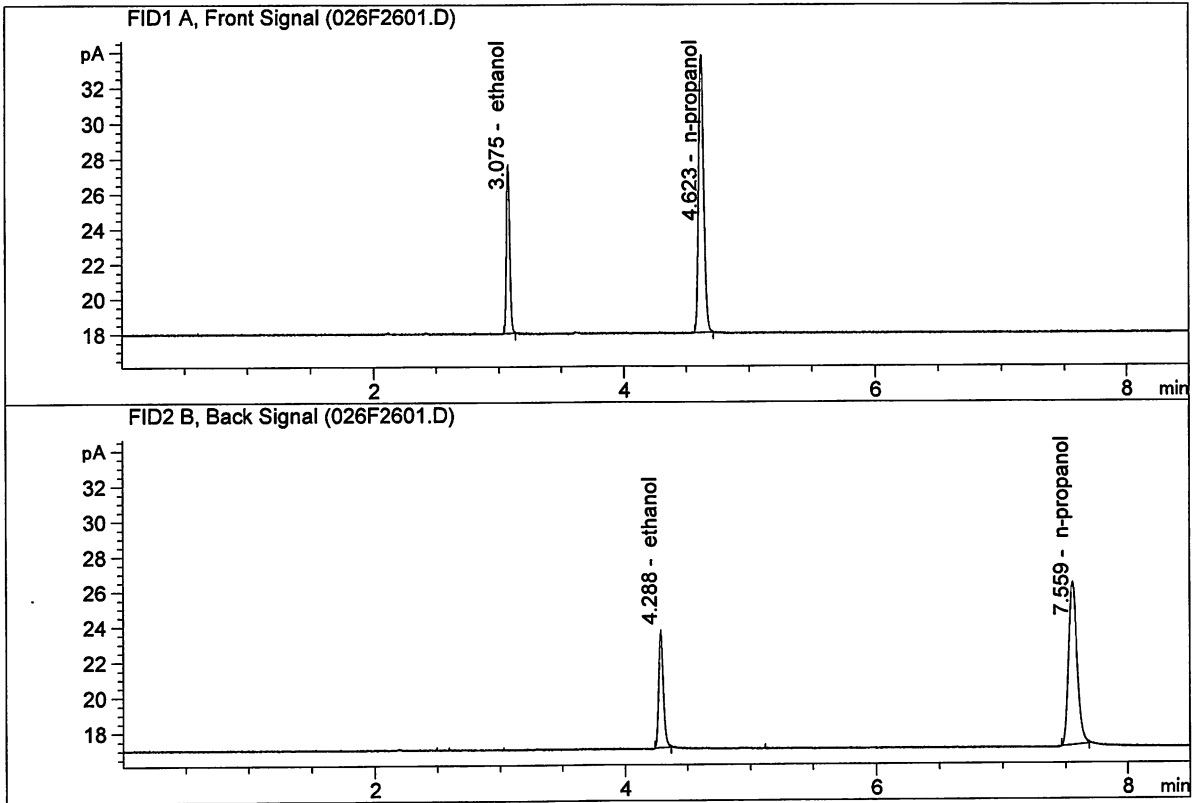

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	17.65111	0.1993	g/100cc
2.	Ethanol	Column 2:	17.89449	0.1994	g/100cc
3.	n-Propanol	Column 1:	44.96155	1.0000	g/100cc
4.	n-Propanol	Column 2:	44.46199	1.0000	g/100cc

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC1-2

Analysis Date(s): 14 Jul 2017

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.0808	0.0822	0.0014	0.0815	0.0813	
(g/100cc)	0.0805	0.0820	0.0015	0.0812		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: ALCOHOL.M
Hamilton Auto-Dilutor Serial Number:
MD96BC1382/MD94AM10010

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.081	0.076	0.086	0.005

	Reported Result 0.081	
--	-------------------------------------	--

Calibration and control data are stored centrally.

Issued: 12/30/2016


Volatiles BAC Calculation Spreadsheet Rev 4

Issuing Authority: Quality Manager

JG

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-2-A
 Laboratory : Meridian
 Injection Date : Jul 14, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

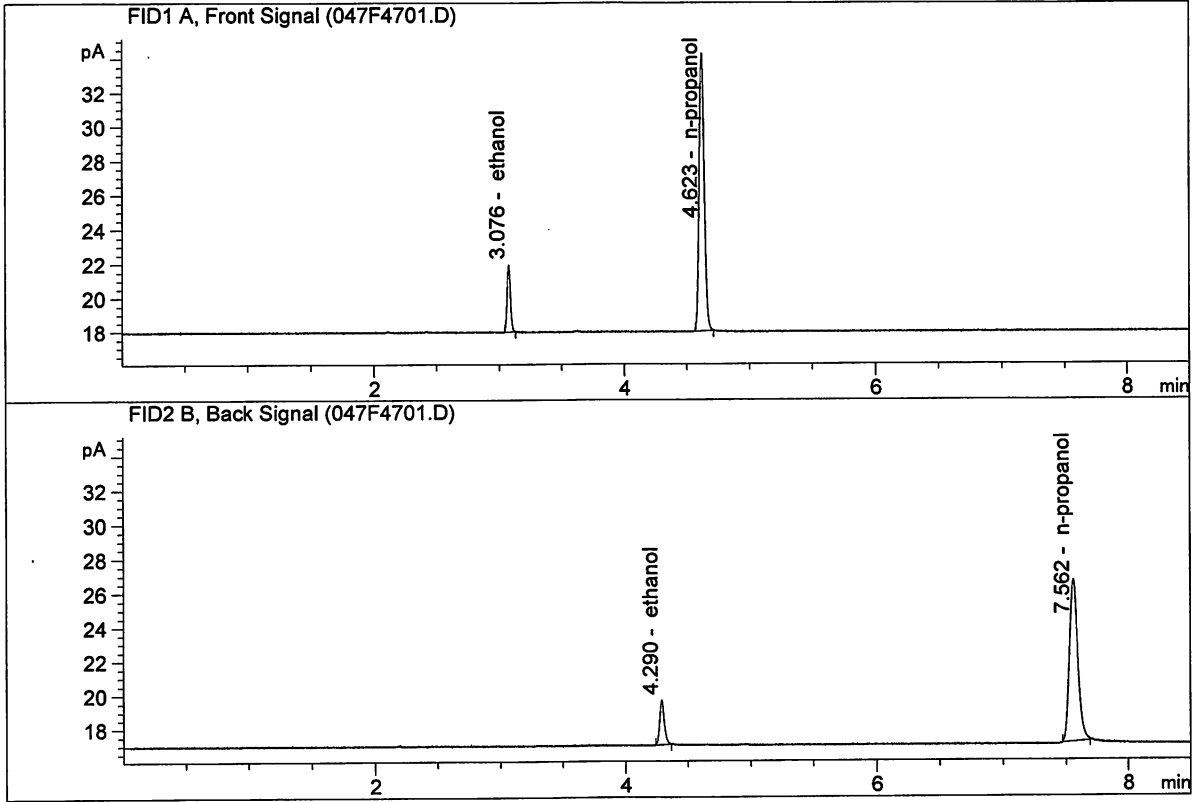


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.28046	0.0808	g/100cc
2.	Ethanol	Column 2:	7.23199	0.0822	g/100cc
3.	n-Propanol	Column 1:	46.30657	1.0000	g/100cc
4.	n-Propanol	Column 2:	45.87421	1.0000	g/100cc

JG

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-2-B
 Laboratory : Meridian
 Injection Date : Jul 14, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

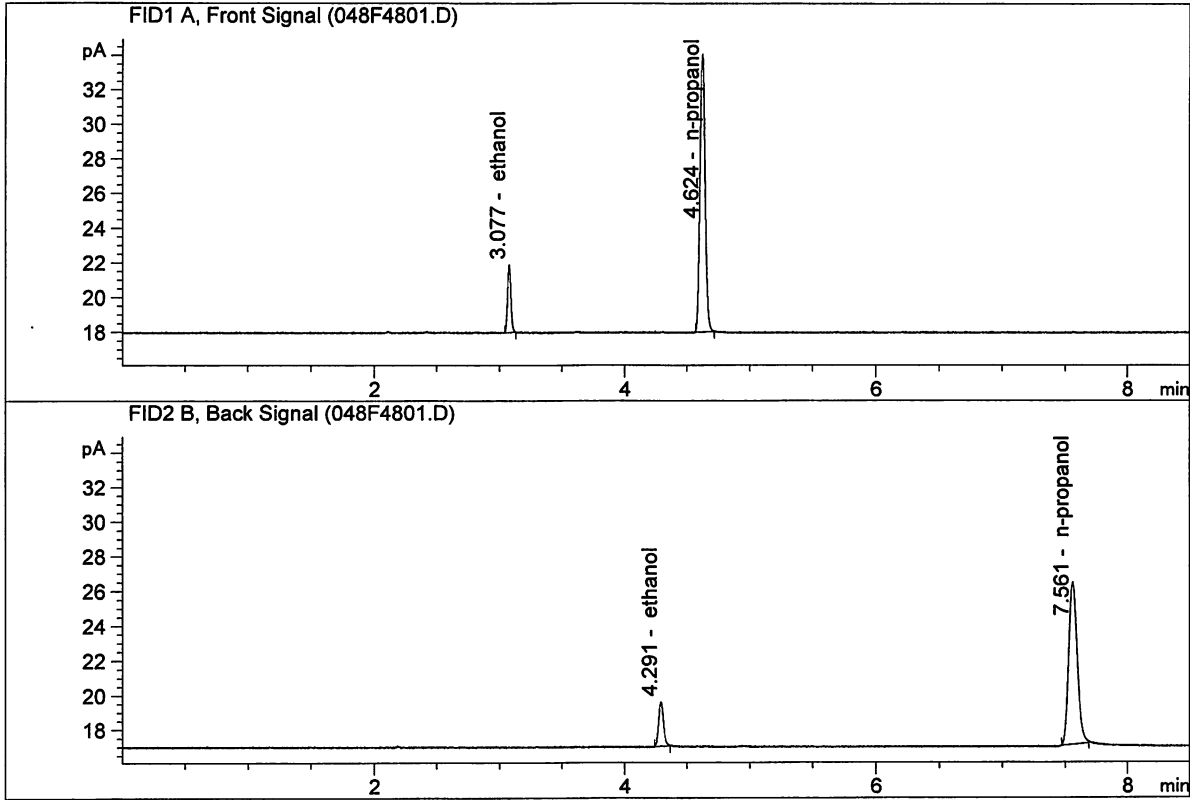

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.16269	0.0805	g/100cc
2.	Ethanol	Column 2:	7.11348	0.0820	g/100cc
3.	n-Propanol	Column 1:	45.71450	1.0000	g/100cc
4.	n-Propanol	Column 2:	45.21114	1.0000	g/100cc

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC2-2

Analysis Date(s): 14 Jul 2017

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.2069	0.2075	0.0006	0.2072	0.2086	
(g/100cc)	0.2099	0.2101	0.0002	0.2100		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: ALCOHOL.M
Hamilton Auto-Dilutor Serial Number:
MD96BC1382/MD94AM10010

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.208	0.197	0.219	0.011

Reported Result	
0.208	

Calibration and control data are stored centrally.

Issued: 12/30/2016


Volatiles BAC Calculation Spreadsheet Rev 4

Issuing Authority: Quality Manager

JG

ISP Forensic Services Blood Alcohol Report

Sample Name : QC2-2-A
 Laboratory : Meridian
 Injection Date : Jul 14, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

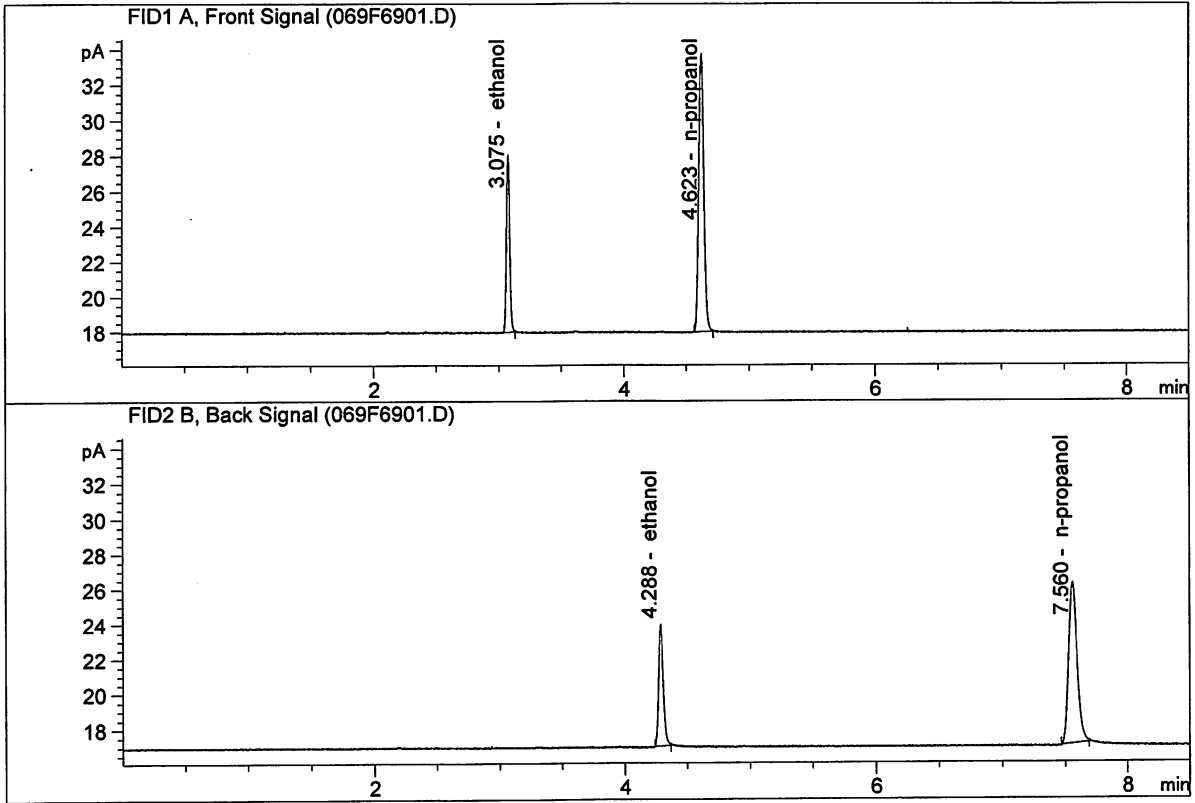


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	18.25713	0.2069	g/100cc
2.	Ethanol	Column 2:	18.51866	0.2075	g/100cc
3.	n-Propanol	Column 1:	44.78499	1.0000	g/100cc
4.	n-Propanol	Column 2:	44.15271	1.0000	g/100cc

JG

ISP Forensic Services Blood Alcohol Report


Sample Name : QC2-2-B
 Laboratory : Meridian
 Injection Date : Jul 14, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

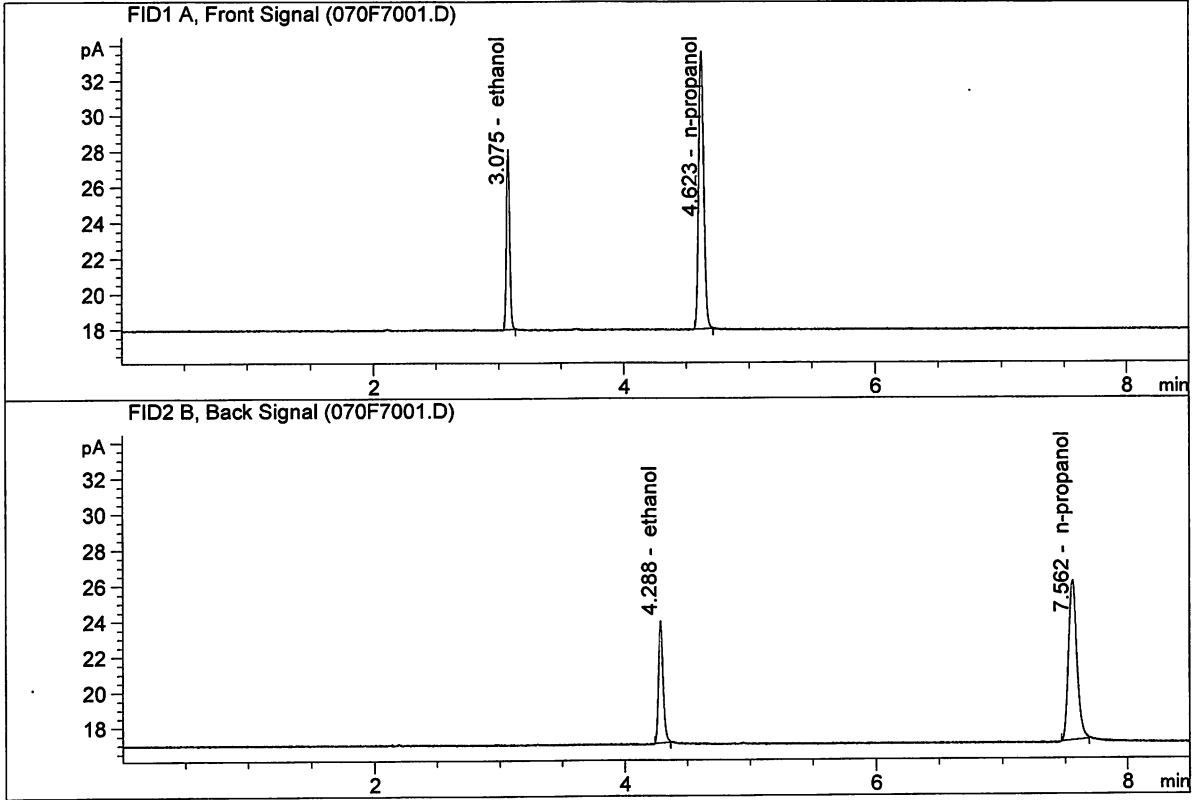

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	18.31698	0.2099	g/100cc
2.	Ethanol	Column 2:	18.53851	0.2101	g/100cc
3.	n-Propanol	Column 1:	44.28193	1.0000	g/100cc
4.	n-Propanol	Column 2:	43.63928	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STD BLK
 Laboratory : Meridian
 Injection Date : Jul 14, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

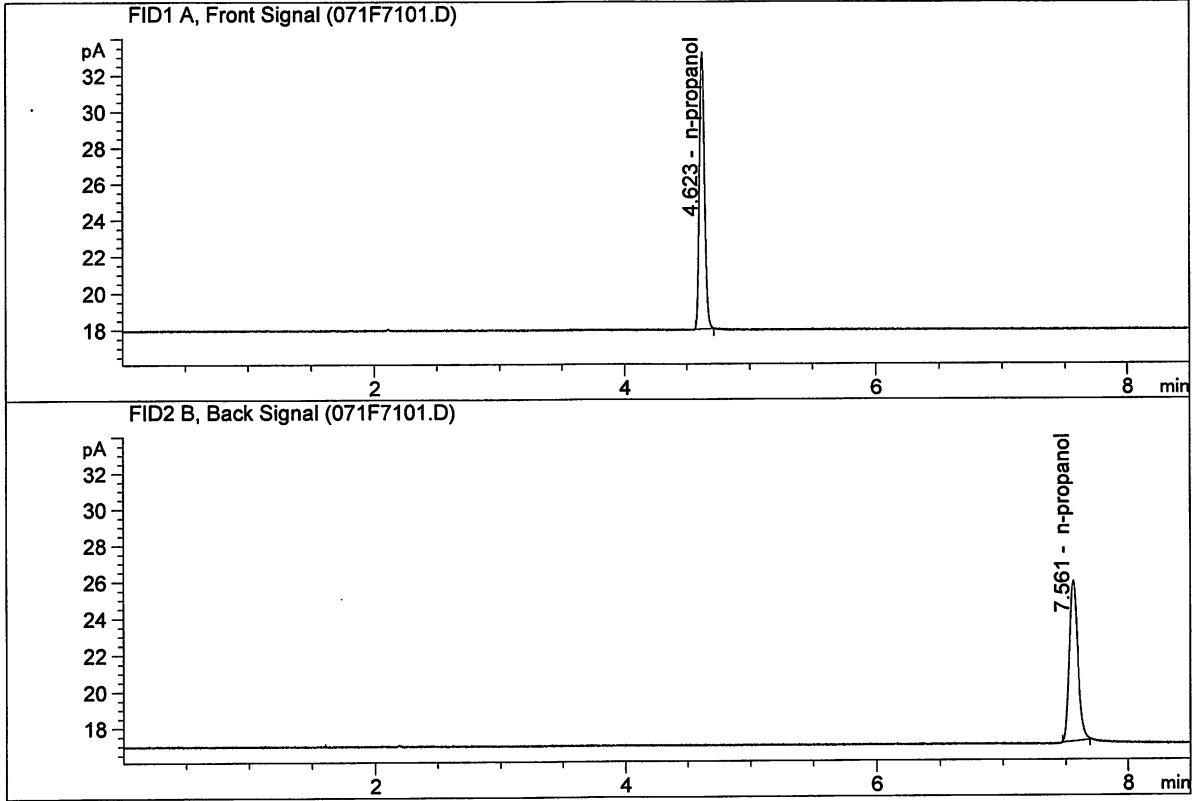

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	43.23688	1.0000	g/100cc
4.	n-Propanol	Column 2:	42.69050	1.0000	g/100cc

UG

S a m p l e S u m m a r y

Sequence table: C:\Chem32\1\Data\07-13-17_SAMPLES\07-13-17_SAMPLES 2017-07-13 16-01-47\07-13-17_SAMPLES.S
 Data directory path: C:\Chem32\1\Data\07-13-17_SAMPLES\07-13-17_SAMPLES 2017-07-13 16-01-47\
 Logbook: C:\Chem32\1\Data\07-13-17_SAMPLES\07-13-17_SAMPLES 2017-07-13 16-01-47\07-13-17_SAMPLES.LOG
 Sequence start: 7/13/2017 4:16:36 PM
 Sequence Operator: SYSTEM
 Operator: SYSTEM
 Method file name: C:\Chem32\1\Data\07-13-17_SAMPLES\07-13-17_SAMPLES 2017-07-13 16-01-47\ALCOHOL.M

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #	Cmp
1	1	1	INTERNAL STD BLK	-	1.0000	001F0101.D		2
2	2	1	MIX VOL FN092314	-	1.0000	002F0201.D		10
3	3	1	QC1-1-A	-	1.0000	003F0301.D		4
4	4	1	QC1-1-B	-	1.0000	004F0401.D		4
5	5	1	0.08 FN10281510-	-	1.0000	005F0501.D		4
6	6	1	0.08 FN10281510-	-	1.0000	006F0601.D		4
7	7	1	M2017-3013-1-A	-	1.0000	007F0701.D		4
8	8	1	M2017-3013-1-B	-	1.0000	008F0801.D		4
9	9	1	M2017-3059-1-A	-	1.0000	009F0901.D		4
10	10	1	M2017-3059-1-B	-	1.0000	010F1001.D		4
11	11	1	M2017-3060-1-A	-	1.0000	011F1101.D		4
12	12	1	M2017-3060-1-B	-	1.0000	012F1201.D		4
13	13	1	M2017-3061-1-A	-	1.0000	013F1301.D		4
14	14	1	M2017-3061-1-B	-	1.0000	014F1401.D		4
15	15	1	M2017-3063-1-A	-	1.0000	015F1501.D		4
16	16	1	M2017-3063-1-B	-	1.0000	016F1601.D		4
17	17	1	M2017-3066-1-A	-	1.0000	017F1701.D		4
18	18	1	M2017-3066-1-B	-	1.0000	018F1801.D		4
19	19	1	M2017-3072-1-A	-	1.0000	019F1901.D		4
20	20	1	M2017-3072-1-B	-	1.0000	020F2001.D		4
21	21	1	M2017-3082-1-A	-	1.0000	021F2101.D		2
22	22	1	M2017-3082-1-B	-	1.0000	022F2201.D		2
23	23	1	M2017-3089-1-A	-	1.0000	023F2301.D		4
24	24	1	M2017-3089-1-B	-	1.0000	024F2401.D		4
25	25	1	QC2-1-A	-	1.0000	025F2501.D		4
26	26	1	QC2-1-B	-	1.0000	026F2601.D		4
27	27	1	M2017-3090-1-A	-	1.0000	027F2701.D		2
28	28	1	M2017-3090-1-B	-	1.0000	028F2801.D		2
29	29	1	M2017-3091-1-A	-	1.0000	029F2901.D		2
30	30	1	M2017-3091-1-B	-	1.0000	030F3001.D		2
31	31	1	M2017-3092-1-A	-	1.0000	031F3101.D		4
32	32	1	M2017-3092-1-B	-	1.0000	032F3201.D		4
33	33	1	M2017-3103-1-A	-	1.0000	033F3301.D		2
34	34	1	M2017-3103-1-B	-	1.0000	034F3401.D		2
35	35	1	M2017-3112-1-A	-	1.0000	035F3501.D		4
36	36	1	M2017-3112-1-B	-	1.0000	036F3601.D		4
37	37	1	M2017-3113-1-A	-	1.0000	037F3701.D		4
38	38	1	M2017-3113-1-B	-	1.0000	038F3801.D		4
39	39	1	M2017-3151-1-A	-	1.0000	039F3901.D		4
40	40	1	M2017-3151-1-B	-	1.0000	040F4001.D		4
41	41	1	M2017-3152-1-A	-	1.0000	041F4101.D		2
42	42	1	M2017-3152-1-B	-	1.0000	042F4201.D		2
43	43	1	M2017-3153-1-A	-	1.0000	043F4301.D		4

56

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal # Cmp
44	44	1	M2017-3153-1-B	-	1.0000	044F4401.D	4
45	45	1	M2017-3157-2-A <i>JG = 3-A</i>	-	1.0000	045F4501.D	2
46	46	1	M2017-3157-2-B <i>JG - 3-A</i>	-	1.0000	046F4601.D	2
47	47	1	QC1-2-A	-	1.0000	047F4701.D	4
48	48	1	QC1-2-B	-	1.0000	048F4801.D	4
49	49	1	M2017-3158-1-A	-	1.0000	049F4901.D	4
50	50	1	M2017-3158-1-B	-	1.0000	050F5001.D	4
51	51	1	M2017-3159-1-A	-	1.0000	051F5101.D	4
52	52	1	M2017-3159-1-B	-	1.0000	052F5201.D	4
53	53	1	M2017-3160-1-A	-	1.0000	053F5301.D	2
54	54	1	M2017-3160-1-B	-	1.0000	054F5401.D	2
55	55	1	M2017-3161-1-A	-	1.0000	055F5501.D	4
56	56	1	M2017-3161-1-B	-	1.0000	056F5601.D	4
57	57	1	M2017-3162-1-A	-	1.0000	057F5701.D	4
58	58	1	M2017-3162-1-B	-	1.0000	058F5801.D	4
59	59	1	M2017-3182-1-A	-	1.0000	059F5901.D	4
60	60	1	M2017-3182-1-B	-	1.0000	060F6001.D	4
61	61	1	M2017-3194-1-A	-	1.0000	061F6101.D	2
62	62	1	M2017-3194-1-B	-	1.0000	062F6201.D	2
63	63	1	M2017-3195-1-A	-	1.0000	063F6301.D	4
64	64	1	M2017-3195-1-B	-	1.0000	064F6401.D	4
65	65	1	P2017-1380-2-A	-	1.0000	065F6501.D	4
66	66	1	P2017-1380-2-B	-	1.0000	066F6601.D	4
67	67	1	P2017-1428-2-A	-	1.0000	067F6701.D	2
68	68	1	P2017-1428-2-B	-	1.0000	068F6801.D	2
69	69	1	QC2-2-A	-	1.0000	069F6901.D	4
70	70	1	QC2-2-B	-	1.0000	070F7001.D	4
71	71	1	INTERNAL STD BLK	-	1.0000	071F7101.D	2

Method file name: C:\Chem32\1\Data\07-13-17_SAMPLES\07-13-17_SAMPLES 2017-07-13 16-01-47 \SHUTDOWN.M

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal # Cmp
72	72	1	EMPTY	-	1.0000	072F7201.D	0

=====
Calibration Table
=====

General Calibration Setting

Calib. Data Modified : Friday, July 07, 2017 3:08:21 PM
Signals calculated separately : No

Rel. Reference Window : 0.000 %
Abs. Reference Window : 0.100 min
Rel. Non-ref. Window : 0.000 %
Abs. Non-ref. Window : 0.100 min
Uncalibrated Peaks : not reported
Partial Calibration : Yes, identified peaks are recalibrated
Correct All Ret. Times: No, only for identified peaks

Curve Type : Linear
Origin : Ignored
Weight : Equal

Recalibration Settings:
Average Response : Average all calibrations
Average Retention Time: Floating Average New 75%

Calibration Report Options :
Printout of recalibrations within a sequence:
 Calibration Table after Recalibration
 Normal Report after Recalibration
If the sequence is done with bracketing:
 Results of first cycle (ending previous bracket)

Default Sample ISTD Information (if not set in sample table):

ISTD #	ISTD Amount [g/100cc]	Name
1	1.00000	n-propanol
2	1.00000	n-propanol

Signal Details

Signal 1: FID1 A, Front Signal
Signal 2: FID2 B, Back Signal

Overview Table

JG

RT	Sig	Lvl	Amount [g/100cc]	Area	Rsp.Factor	Ref	ISTD #	Compound
2.586	1	1	1.00000	3.69669	2.70512e-1	No	No 1	methanol
3.072	1	1	5.00000e-2	4.40244	1.13573e-2	No	No 1	ethanol
		2	1.00000e-1	8.85186	1.12971e-2			
		3	2.00000e-1	17.77598	1.12511e-2			
		4	3.00000e-1	26.27114	1.14194e-2			
		5	5.00000e-1	44.13909	1.13278e-2			
3.388	2	1	1.00000	4.26062	2.34707e-1	No	No 2	methanol
3.628	1	1	1.00000	9.73055	1.02769e-1	No	No 1	isopropyl alcohol
4.281	2	1	5.00000e-2	4.38778	1.13953e-2	No	No 2	ethanol
		2	1.00000e-1	8.85360	1.12948e-2			
		3	2.00000e-1	18.10852	1.10445e-2			
		4	3.00000e-1	26.94650	1.11332e-2			
		5	5.00000e-1	45.78714	1.09201e-2			
4.308	1	1	1.00000	6.49940	1.53860e-1	No	No 1	acetone
4.618	1	1	1.00000	45.03209	2.22064e-2	No	Yes 1	n-propanol
		2	1.00000	45.43357	2.20102e-2			
		3	1.00000	45.32043	2.20651e-2			
		4	1.00000	44.32218	2.25621e-2			
		5	1.00000	44.57899	2.24321e-2			
4.661	2	1	1.00000	6.89301	1.45075e-1	No	No 2	acetone
4.969	2	1	1.00000	10.70642	9.34019e-2	No	No 2	isopropyl alcohol
7.550	2	1	1.00000	45.56691	2.19458e-2	No	Yes 2	n-propanol
		2	1.00000	45.69565	2.18839e-2			
		3	1.00000	45.41307	2.20201e-2			
		4	1.00000	44.22663	2.26108e-2			
		5	1.00000	44.27934	2.25839e-2			


Peak Sum Table

No Entries in table

1 Warnings or Errors :


Warning : Curve requires more calibration points., (methanol)

Calibration Curves

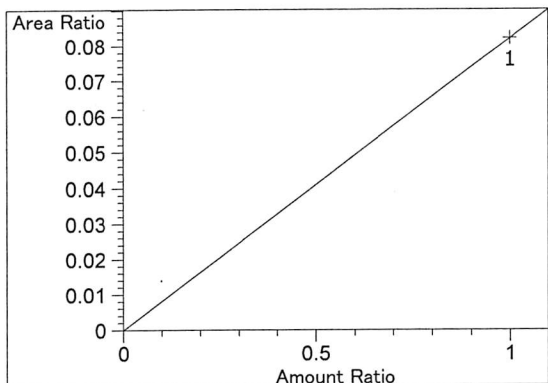


methanol at exp. RT: 2.586
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 8.20902e-2
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio


56

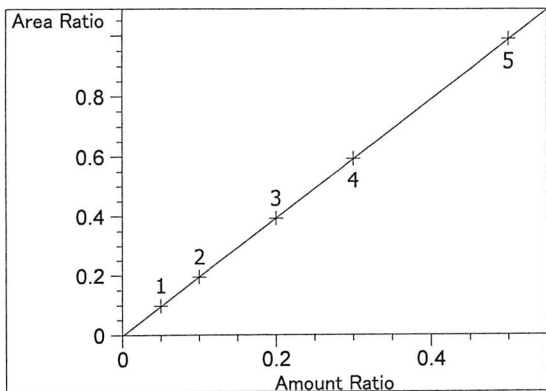


ethanol at exp. RT: 3.072
 FID1 A, Front Signal
 Correlation: 0.99999
 Residual Std. Dev.: 0.00145
 Formula: $y = mx + b$
 m: 1.98543
 b: -3.11136e-3
 x: Amount Ratio
 y: Area Ratio

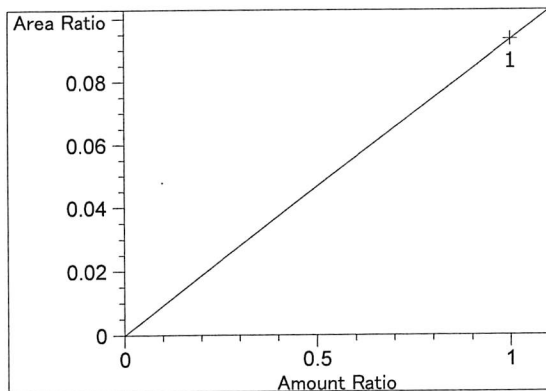

methanol at exp. RT: 3.388
 FID2 B, Back Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 9.35026e-2
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio

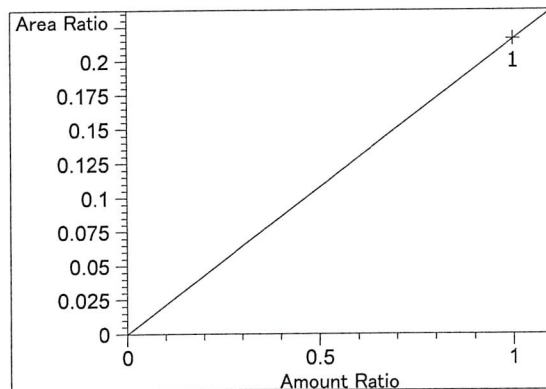


isopropyl alcohol at exp. RT: 3.628
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 2.16080e-1
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio

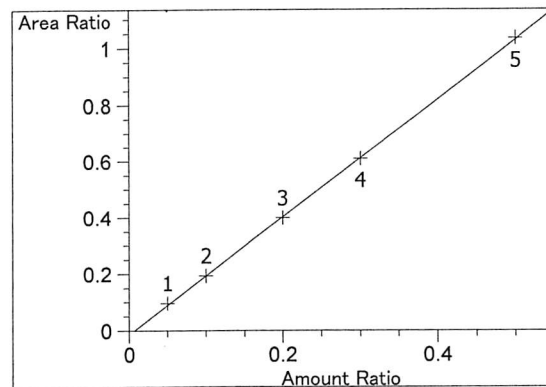


ethanol at exp. RT: 4.281
 FID2 B, Back Signal
 Correlation: 0.99992
 Residual Std. Dev.: 0.00533
 Formula: $y = mx + b$
 m: 2.08876
 b: -1.39879e-2
 x: Amount Ratio
 y: Area Ratio


JG

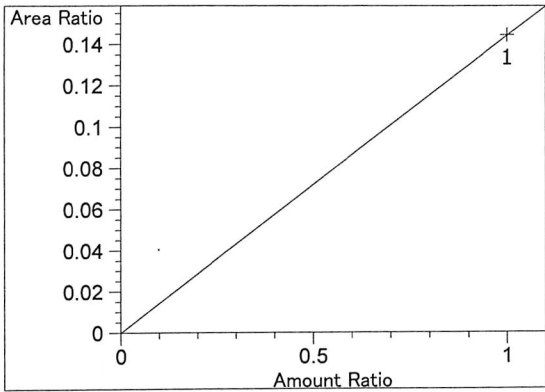


acetone at exp. RT: 4.308
FID1 A, Front Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx + b$
m: 1.44328e-1
b: 0.00000
x: Amount Ratio
y: Area Ratio

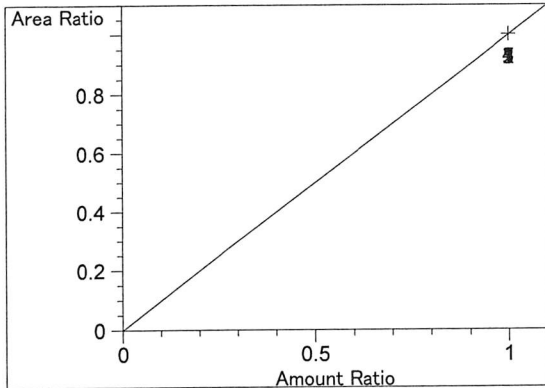

n-propanol at exp. RT: 4.618
FID1 A, Front Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx + b$
m: 1.00000
b: 0.00000
x: Amount Ratio
y: Area Ratio

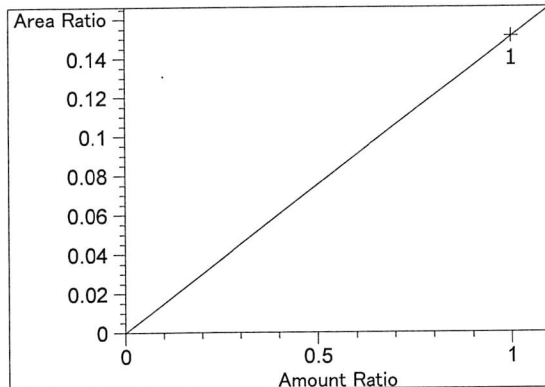


acetone at exp. RT: 4.661
FID2 B, Back Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx + b$
m: 1.51272e-1
b: 0.00000
x: Amount Ratio
y: Area Ratio

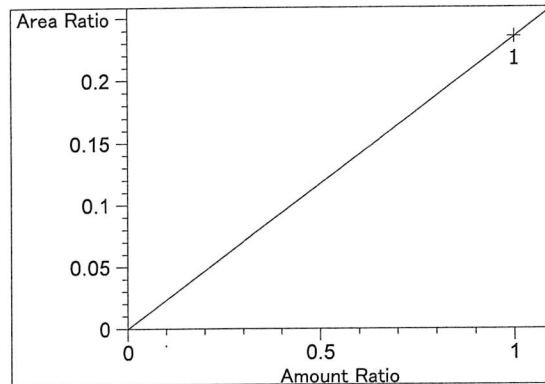

isopropyl alcohol at exp. RT: 4.969
FID2 B, Back Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx + b$
m: 2.34960e-1
b: 0.00000
x: Amount Ratio
y: Area Ratio

JG

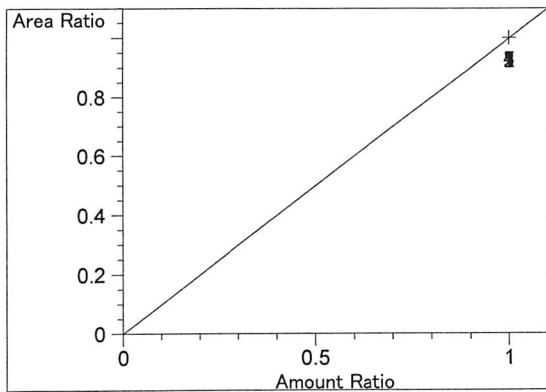


n-propanol at exp. RT: 7.550
FID2 B, Back Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx + b$
m: 1.00000
b: 0.00000
x: Amount Ratio
y: Area Ratio

=====

JG

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.050 FN06231406
 Laboratory : Meridian
 Injection Date : Jul 7, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

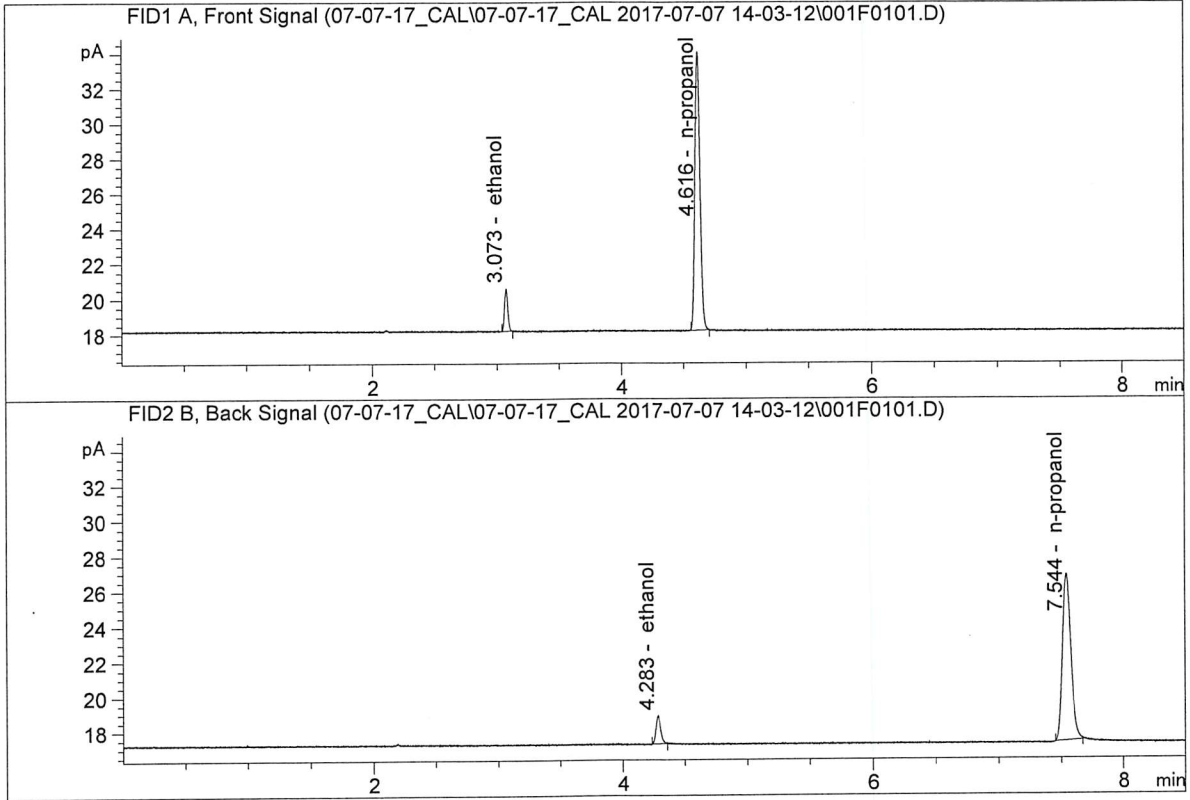


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	4.40244	0.0508	g/100cc
2.	Ethanol	Column 2:	4.38778	0.0528	g/100cc
3.	n-Propanol	Column 1:	45.03209	1.0000	g/100cc
4.	n-Propanol	Column 2:	45.56691	1.0000	g/100cc

JG

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.100 FN06181501
 Laboratory : Meridian
 Injection Date : Jul 7, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

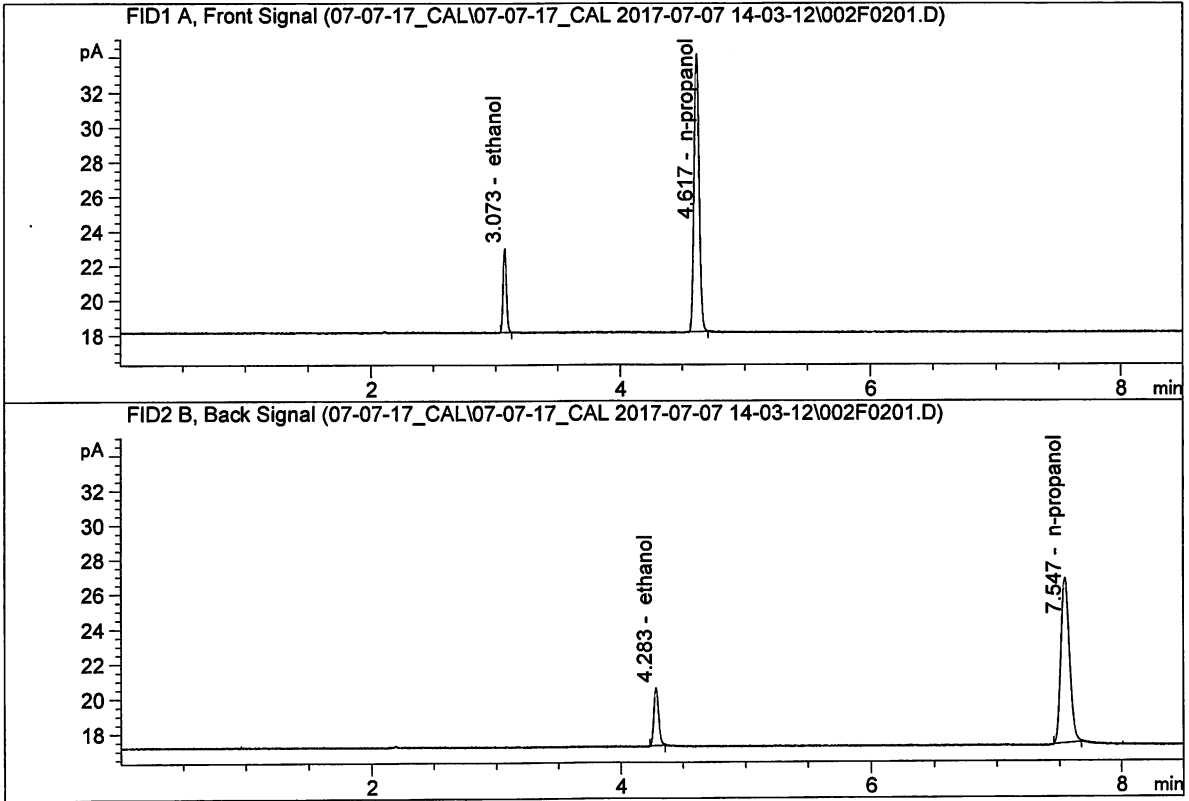


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	8.85186	0.0997	g/100cc
2.	Ethanol	Column 2:	8.85360	0.0995	g/100cc
3.	n-Propanol	Column 1:	45.43357	1.0000	g/100cc
4.	n-Propanol	Column 2:	45.69565	1.0000	g/100cc

56

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.200 FN07201502
 Laboratory : Meridian
 Injection Date : Jul 7, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

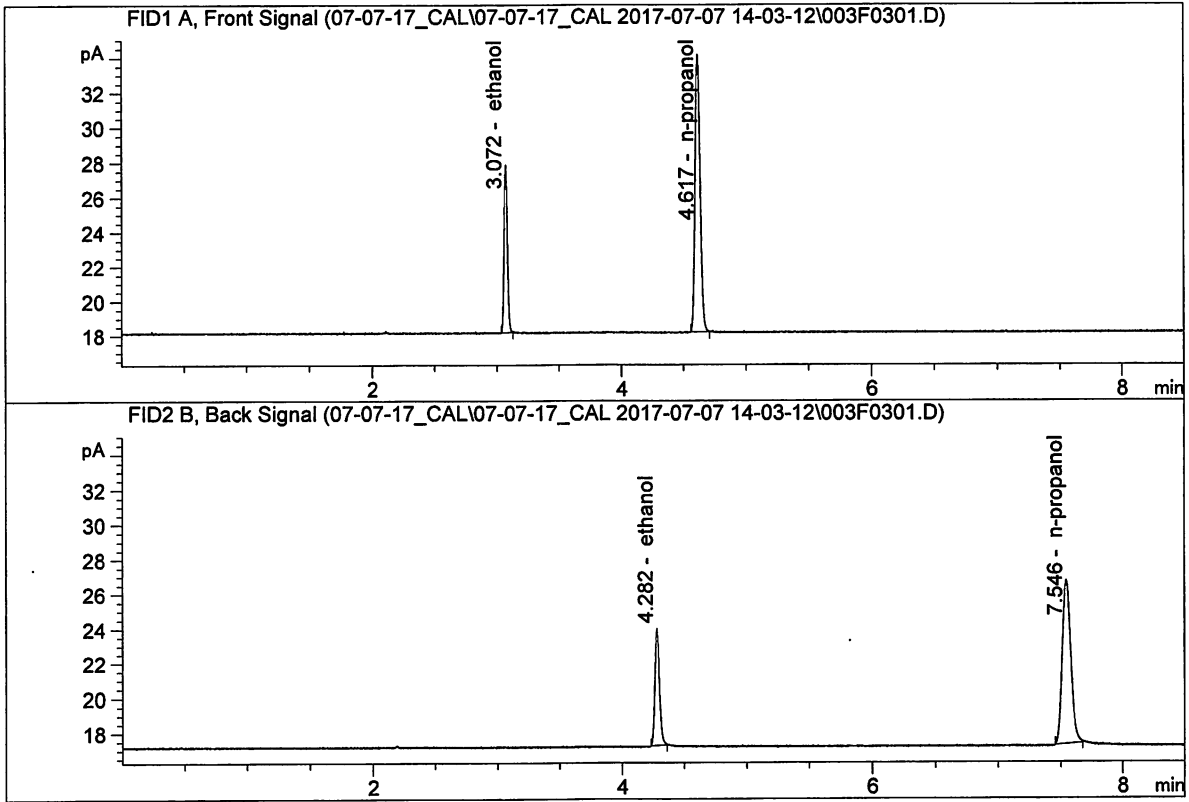


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	17.77598	0.1991	g/100cc
2.	Ethanol	Column 2:	18.10852	0.1976	g/100cc
3.	n-Propanol	Column 1:	45.32043	1.0000	g/100cc
4.	n-Propanol	Column 2:	45.41307	1.0000	g/100cc

JG

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.300 FN02121601
 Laboratory : Meridian
 Injection Date : Jul 7, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

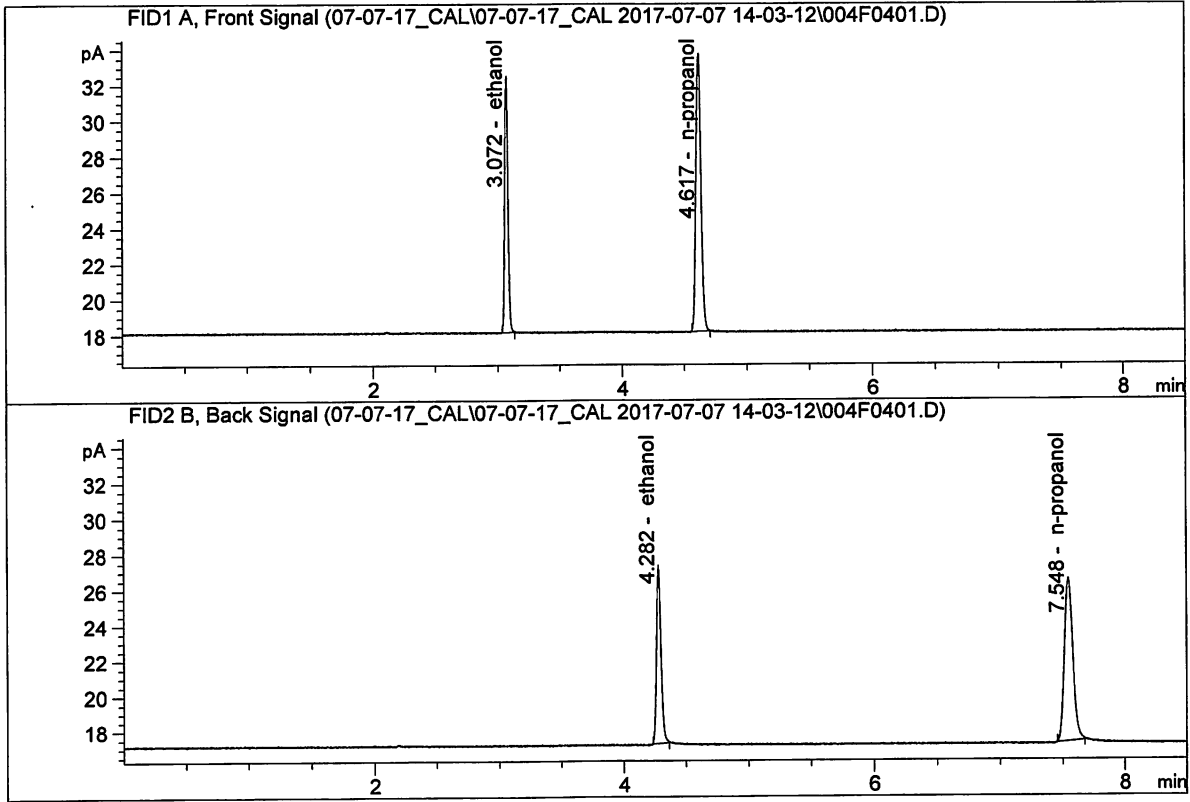


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	26.27114	0.3001	g/100cc
2.	Ethanol	Column 2:	26.94650	0.2984	g/100cc
3.	n-Propanol	Column 1:	44.32218	1.0000	g/100cc
4.	n-Propanol	Column 2:	44.22663	1.0000	g/100cc

JG

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.500 FN07031402
 Laboratory : Meridian
 Injection Date : Jul 7, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

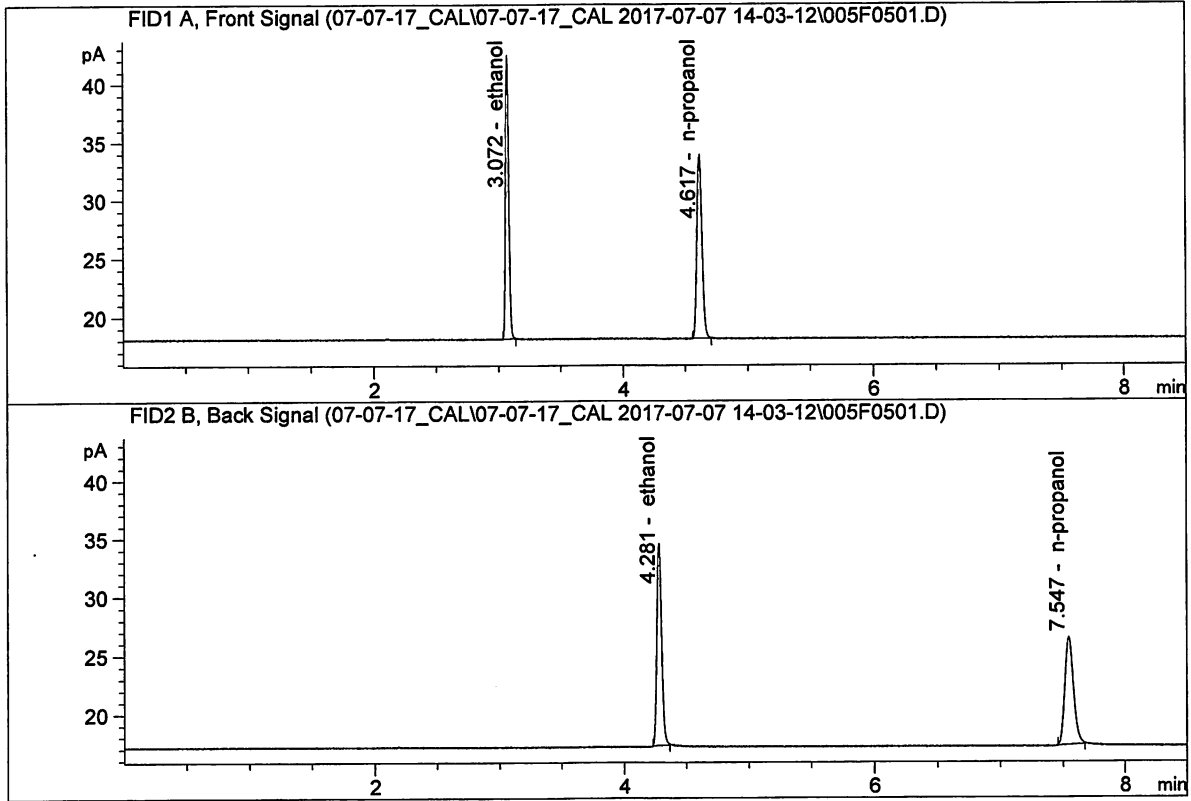


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	44.13909	0.5003	g/100cc
2.	Ethanol	Column 2:	45.78714	0.5018	g/100cc
3.	n-Propanol	Column 1:	44.57899	1.0000	g/100cc
4.	n-Propanol	Column 2:	44.27934	1.0000	g/100cc

JG

ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STANDARD BLANK
 Laboratory : Meridian
 Injection Date : Jul 7, 2017
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

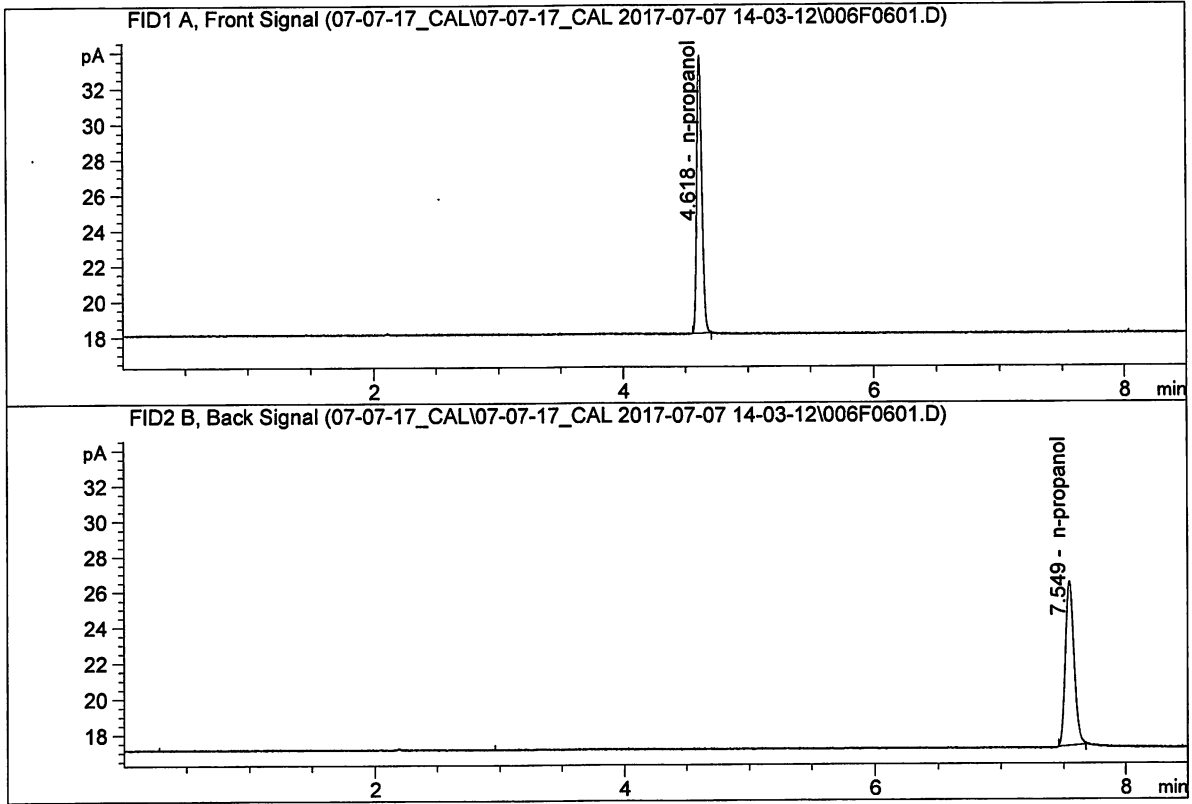

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	44.17977	1.0000	g/100cc
4.	n-Propanol	Column 2:	44.10345	1.0000	g/100cc

UG