

**REVIEWED**

By Rachel Cutler at 10:08 am, Dec 23, 2018

**Quantitative Analysis for Ethanol & Qualitative Analysis for Other Volatiles**

*Analytical Method(s): 1.0*

**Device: Hamilton MICROLAB 600 Liquid Processor/Dilutor Serial Number: ML600HC11378**

**Volatiles Quality Assurance Controls**

**Run Date: 12/19/18-12/20/18**  
Calibration Date: 12/11/18

Control level	Expiration	Lot #	Target Value	Acceptable Range	Overall Results
Level 1	Jan-22	1801036	0.0812	0.0731-0.0893	0.0774 g/100cc 0.0803 g/100cc g/100cc
Level 2	Mar-22	1803028	0.2035	0.1832-0.2238	0.2015 g/100cc 0.2121 g/100cc g/100cc
<b>Multi-Component mixture:</b>		<b>Exp date: Sept. 2020</b>	<b>Lot #</b>	<b>FN06041502</b>	<b>OK</b>
<b>Curve Fit:</b>		<b>Column 1</b>	<b>1.00000</b>	<b>Column 2</b>	<b>0.99994</b>

**Ethanol Calibration Reference Material**

Calibrator level	Expiration	Cerilliant Lot #	Target Value	Acceptable Range	Column 1	Column 2	Precision	Mean
0.050	Jul-19	FN06231406	0.050	0.045 - 0.055	0.0505	0.0520	0.0015	0.0512
0.080			0.080	0.072 - 0.088			0	#DIV/0!
0.100	Aug-21	FN08101601	0.100	0.090 - 0.110	0.0998	0.1003	0.0005	0.1
0.200	Dec-19	FN12011401	0.200	0.180 - 0.220	0.1997	0.1976	0.0021	0.1986
0.300	Feb-21	FN02121601	0.300	0.270 - 0.330	0.2997	0.2984	0.0013	0.299
0.400			0.400	0.360 - 0.440			0	#DIV/0!
0.500	Sep-21	FN08031602	0.500	0.450 - 0.550	0.5003	0.5016	0.0013	0.5009

**Aqueous Controls**

Control level	Expiration	Cerilliant Lot #	Target Value	Acceptable Range	Overall Results
0.080	May-22	FN04171701	0.08000	0.076 - 0.084	0.080 g/100cc

Issued: 4/22/2015

















~Any information on this document can be changed for laboratory use, except for the precision and mean determination formulas.

Volatiles QA/QC data spreadsheet Rev 5

Issuing Authority: Quality Manager

JCS


**Worklist: 2850**

<u>LAB CASE</u>	<u>ITEM</u>	<u>TASK ID</u>	<u>DESCRIPTION</u>	
M2018-6049	2	134140	Alcohol Analysis	
M2018-6057	1	133751	Alcohol Analysis	
M2018-6071	1	134098	Alcohol Analysis	
M2018-6072	1	134099	Alcohol Analysis	
M2018-6073	1	134100	Alcohol Analysis	
M2018-6074	1	134104	Alcohol Analysis	
M2018-6092	1	134150	Alcohol Analysis	
M2018-6110	1	134252	Alcohol Analysis	
M2018-6111	1	134253	Alcohol Analysis	
M2018-6112	1	134255	Alcohol Analysis	
M2018-6113	1	134256	Alcohol Analysis	
M2018-6128	1	134489	Alcohol Analysis	
M2018-6129	1	134493	Alcohol Analysis	
M2018-6130	1	134497	Alcohol Analysis	
M2018-6134	1	134507	Alcohol Analysis	
M2018-6140	1	134542	Alcohol Analysis	
M2018-6143	1	134546	Alcohol Analysis	
M2018-6156	1	134723	Alcohol Analysis	
M2018-6160	1	134749	Alcohol Analysis	
M2018-6167	1	134762	Alcohol Analysis	
M2018-6168	1	134763	Alcohol Analysis	
M2018-6170	1	134776	Alcohol Analysis	
M2018-6171	1	134777	Alcohol Analysis	

36


**Worklist: 2850**

<u>LAB CASE</u>	<u>ITEM</u>	<u>TASK ID</u>	<u>DESCRIPTION</u>
M2018-6172	1	134781	Alcohol Analysis
P2018-3413	2	133828	Alcohol Analysis
P2018-3422	1	133554	Alcohol Analysis
P2018-3423	1	133558	Alcohol Analysis

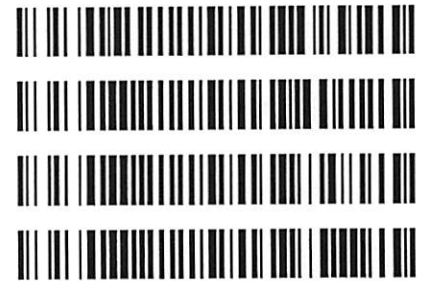

ISP Forensic Services Blood Alcohol Report


Sample Name : INTERNAL STD BLK 1  
 Laboratory : Meridian  
 Injection Date : Dec 19, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

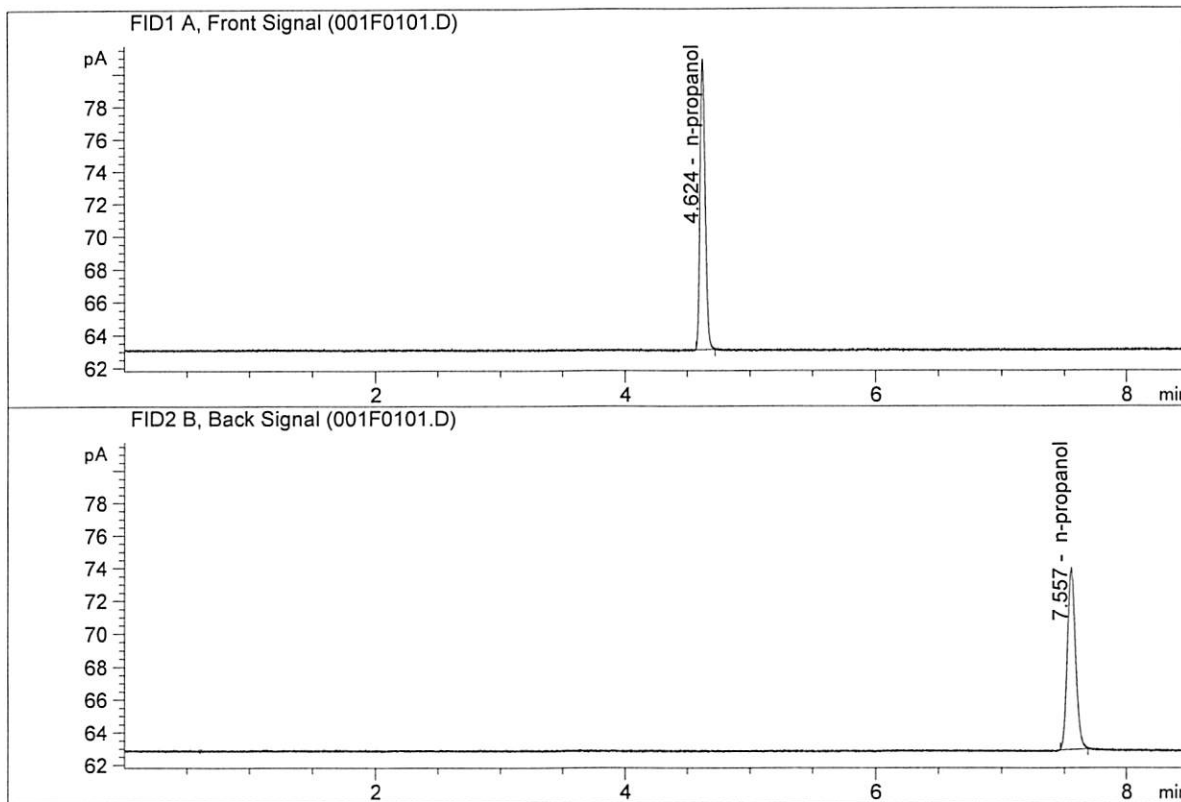

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	50.61840	1.0000	g/100cc
4.	n-Propanol	Column 2:	52.99815	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report

Sample Name : MIX VOL FN06041502  
 Laboratory : Meridian  
 Injection Date : Dec 19, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

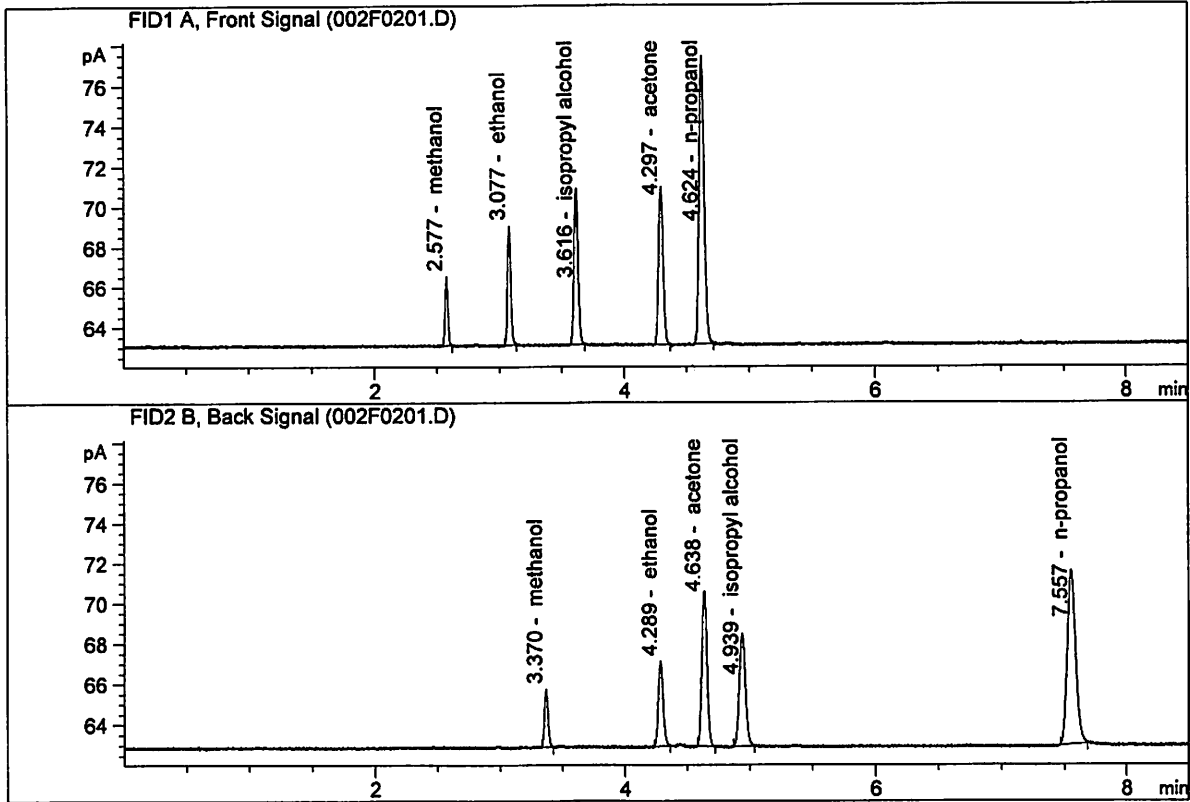

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	10.71027	0.1460	g/100cc
2.	Ethanol	Column 2:	10.99505	0.1457	g/100cc
3.	n-Propanol	Column 1:	40.38224	1.0000	g/100cc
4.	n-Propanol	Column 2:	41.28026	1.0000	g/100cc

JG

## VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC1-1

Analysis Date(s): 19 Dec 2018

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.0779	0.0783	0.0004	0.0781	0.0774	
(g/100cc)	0.0760	0.0774	0.0014	0.0767		

### Analysis Method

Refer to Blood Alcohol Method #1

### Instrument Information

*Instrument method is stored centrally.*

Refer to Instrument Method: ALCOHOL.M  
Hamilton Auto-Dilutor Serial Number: ML600HC11378

### Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.077	0.073	0.081	0.004

	<b>Reported Result</b>	
	0.077	

*Calibration and control data are stored centrally.*


Issued: 12/30/2016

Volatiles BAC Calculation Spreadsheet Rev 4

Issuing Authority: Quality Manager

ISP Forensic Services Blood Alcohol Report


Sample Name : QC1-1-A  
 Laboratory : Meridian  
 Injection Date : Dec 19, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

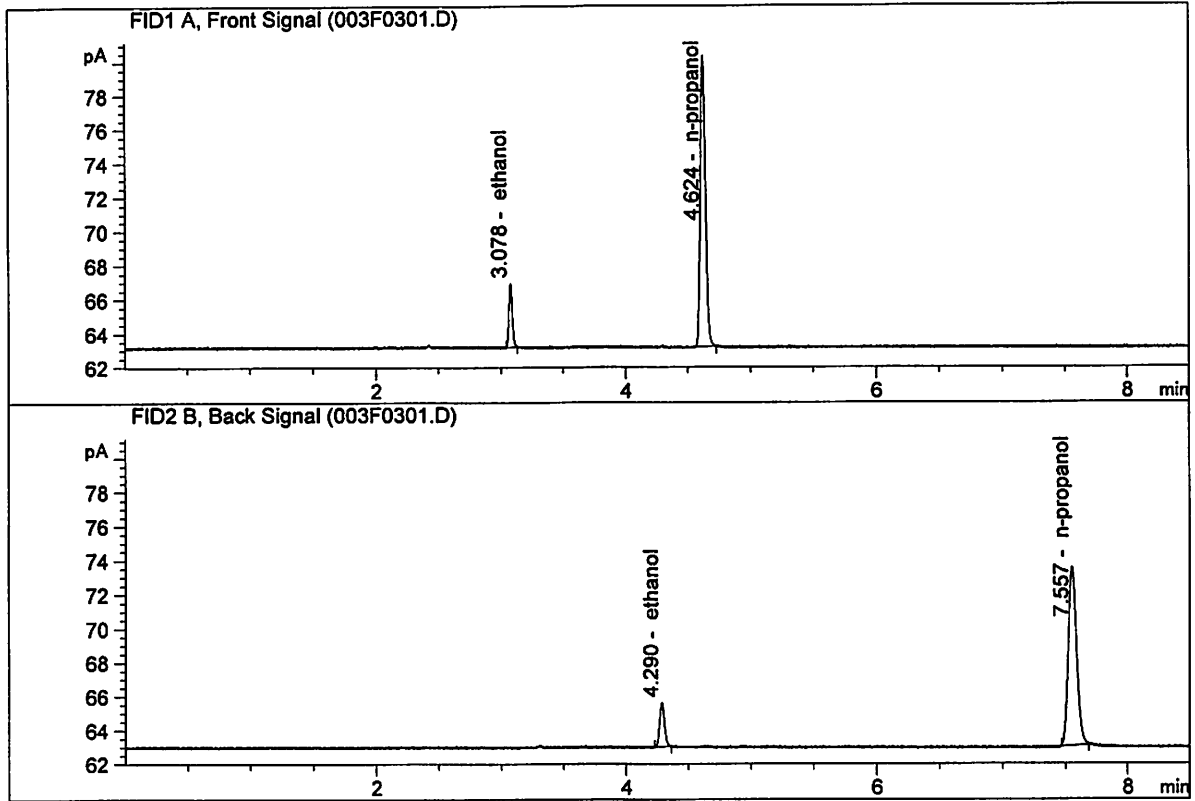

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	6.85668	0.0779	g/100cc
2.	Ethanol	Column 2:	6.94388	0.0783	g/100cc
3.	n-Propanol	Column 1:	48.84159	1.0000	g/100cc
4.	n-Propanol	Column 2:	50.11260	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-1-B  
 Laboratory : Meridian  
 Injection Date : Dec 19, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

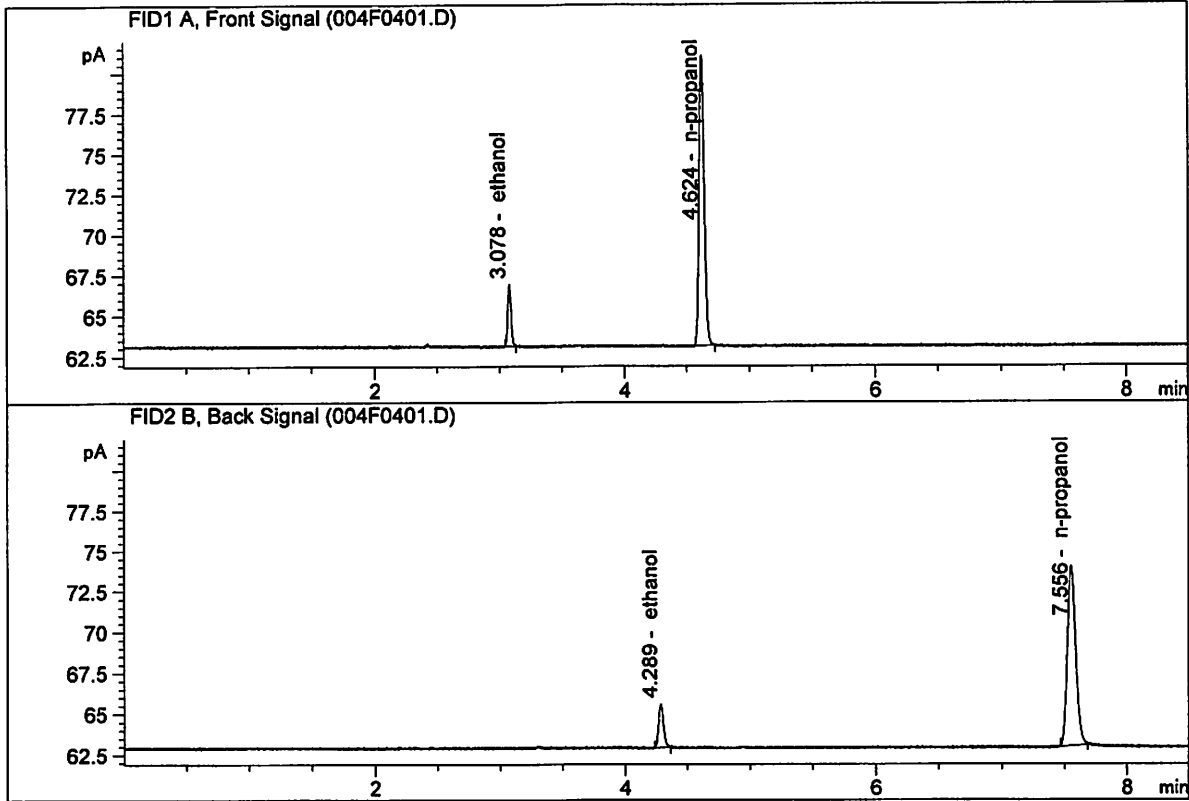

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	6.99164	0.0760	g/100cc
2.	Ethanol	Column 2:	7.19041	0.0774	g/100cc
3.	n-Propanol	Column 1:	51.06061	1.0000	g/100cc
4.	n-Propanol	Column 2:	52.51464	1.0000	g/100cc



# VOLATILES DETERMINATION CASEFILE WORKSHEET

**Laboratory No.: 0.08 FN04171701**

**Analysis Date(s): 19 Dec 2018**

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.0804	0.0799	0.0005	0.0801	0.0804	
(g/100cc)	0.0808	0.0807	0.0001	0.0807		

**Analysis Method**

Refer to Blood Alcohol Method #1

**Instrument Information**

*Instrument method is stored centrally.*

Refer to Instrument Method: ALCOHOL.M  
Hamilton Auto-Dilutor Serial Number: ML600HC11378

**Reporting of Results**

**Uncertainty of Measurement (UM%): 5.00%**

Overall Mean (g/100cc)	Low	High	5% of Mean
0.080	0.076	0.084	0.004

	<b>Reported Result</b>  0.080	
--	-------------------------------------	--

*Calibration and control data are stored centrally.*

Issued: 12/30/2016


Volatiles BAC Calculation Spreadsheet Rev 4

Issuing Authority: Quality Manager

JG

ISP Forensic Services Blood Alcohol Report


Sample Name : 0.08 FN04171701-A  
 Laboratory : Meridian  
 Injection Date : Dec 19, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

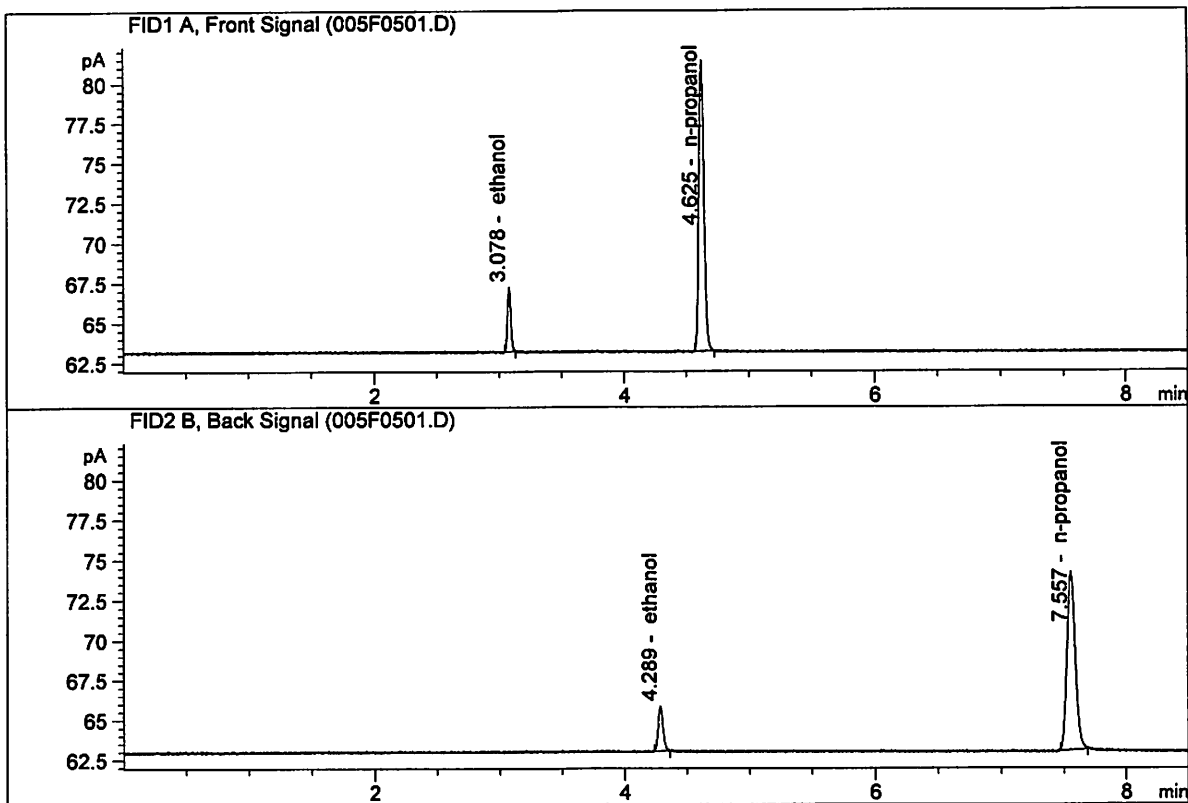

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.48984	0.0804	g/100cc
2.	Ethanol	Column 2:	7.53626	0.0799	g/100cc
3.	n-Propanol	Column 1:	51.67758	1.0000	g/100cc
4.	n-Propanol	Column 2:	53.18303	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.08 FN04171701-B  
 Laboratory : Meridian  
 Injection Date : Dec 19, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

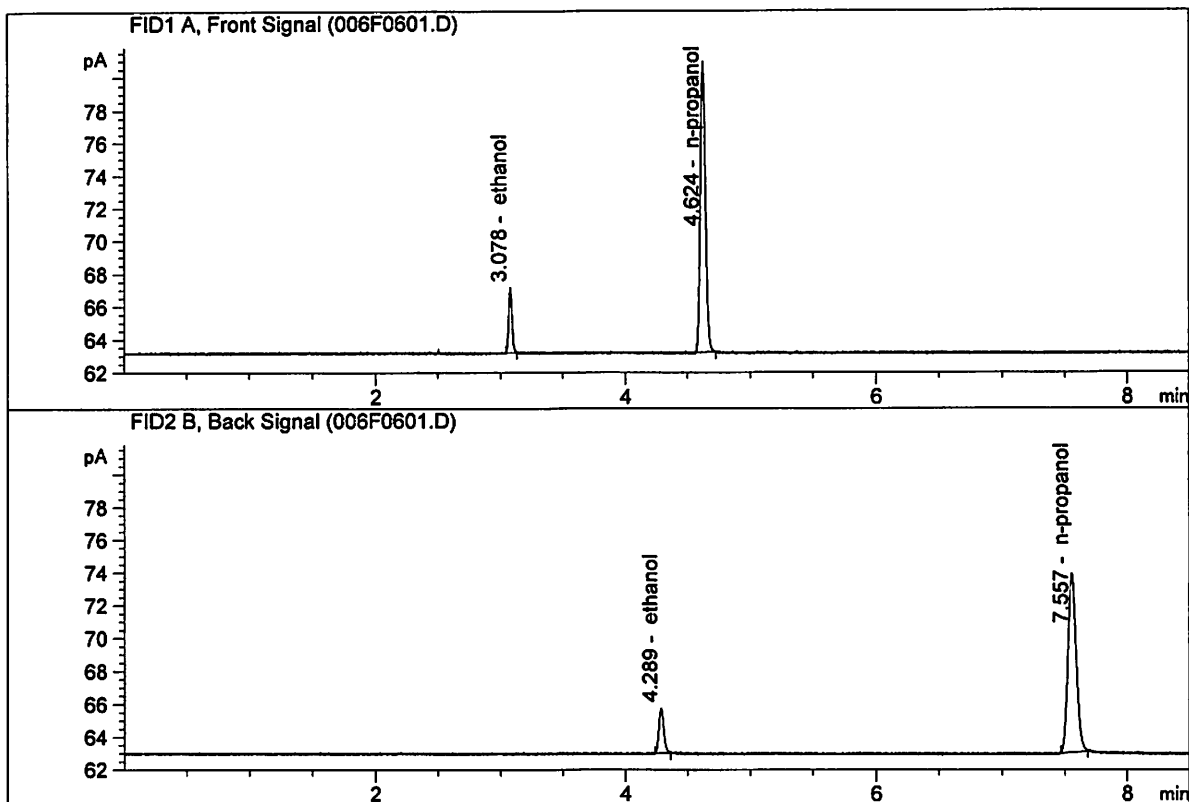

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.35110	0.0808	g/100cc
2.	Ethanol	Column 2:	7.40965	0.0807	g/100cc
3.	n-Propanol	Column 1:	50.46377	1.0000	g/100cc
4.	n-Propanol	Column 2:	51.77009	1.0000	g/100cc

## VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC2-1

Analysis Date(s): 19 Dec 2018

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.2039	0.2023	0.0016	0.2031	0.2015	
(g/100cc)	0.2006	0.1992	0.0014	0.1999		

**Analysis Method**

Refer to Blood Alcohol Method #1

**Instrument Information**

*Instrument method is stored centrally.*

Refer to Instrument Method: ALCOHOL.M  
Hamilton Auto-Dilutor Serial Number: ML600HC11378

**Reporting of Results**

**Uncertainty of Measurement (UM%): 5.00%**

Overall Mean (g/100cc)	Low	High	5% of Mean
0.201	0.190	0.212	0.011

	<b>Reported Result</b>	
	0.201	

*Calibration and control data are stored centrally.*


Issued: 12/30/2016

Volatiles BAC Calculation Spreadsheet Rev 4

Issuing Authority: Quality Manager

ISP Forensic Services Blood Alcohol Report


Sample Name : QC2-1-A  
 Laboratory : Meridian  
 Injection Date : Dec 19, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

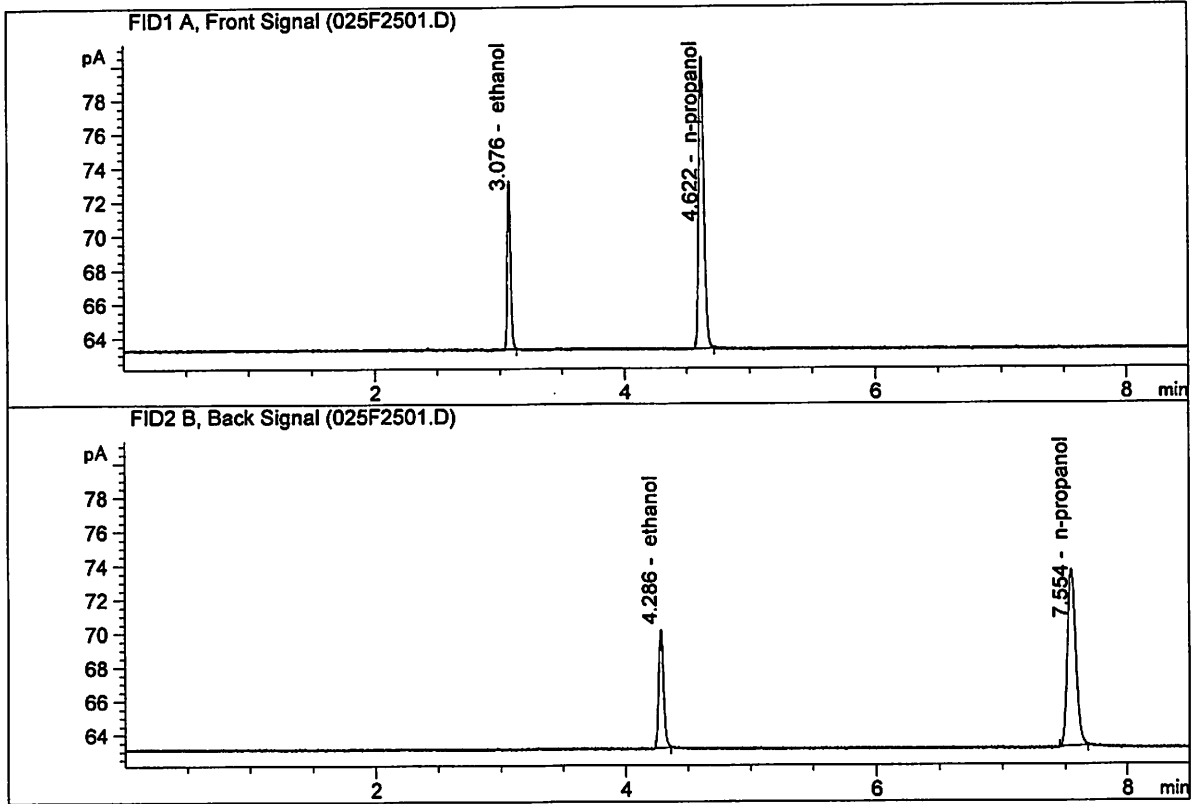

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	18.12546	0.2039	g/100cc
2.	Ethanol	Column 2:	18.65081	0.2023	g/100cc
3.	n-Propanol	Column 1:	48.79264	1.0000	g/100cc
4.	n-Propanol	Column 2:	49.91919	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report

Sample Name : QC2-1-B  
 Laboratory : Meridian  
 Injection Date : Dec 19, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

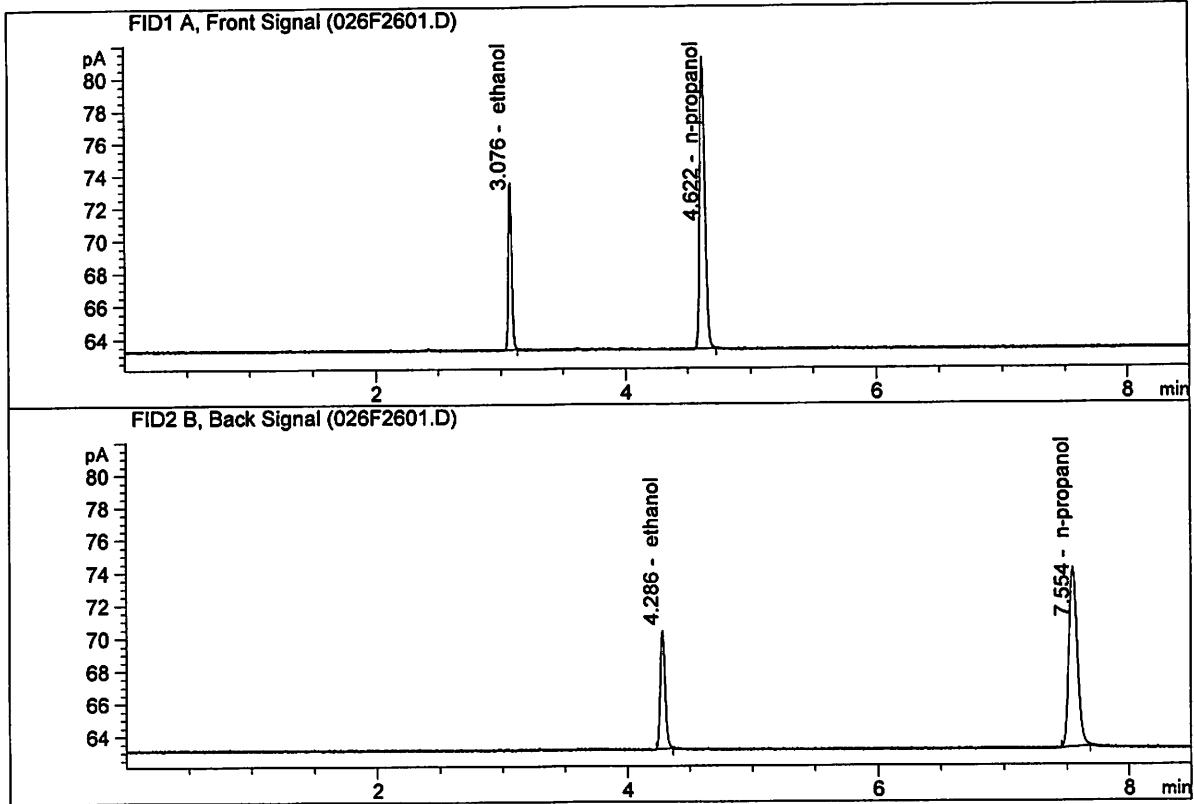

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	18.58604	0.2006	g/100cc
2.	Ethanol	Column 2:	19.19883	0.1992	g/100cc
3.	n-Propanol	Column 1:	50.85109	1.0000	g/100cc
4.	n-Propanol	Column 2:	52.18516	1.0000	g/100cc

## VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC1-2

Analysis Date(s): 19 Dec 2018

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.0798	0.0803	0.0005	0.0800	0.0803	
(g/100cc)	0.0803	0.0809	0.0006	0.0806		

### Analysis Method

Refer to Blood Alcohol Method #1

### Instrument Information

*Instrument method is stored centrally.*

Refer to Instrument Method: ALCOHOL.M  
Hamilton Auto-Dilutor Serial Number: ML600HC11378

### Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.080	0.076	0.084	0.004

	<b>Reported Result</b>	
	0.080	

*Calibration and control data are stored centrally.*


Issued: 12/30/2016

Volatiles BAC Calculation Spreadsheet Rev 4

Issuing Authority: Quality Manager

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-2-A  
 Laboratory : Meridian  
 Injection Date : Dec 19, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

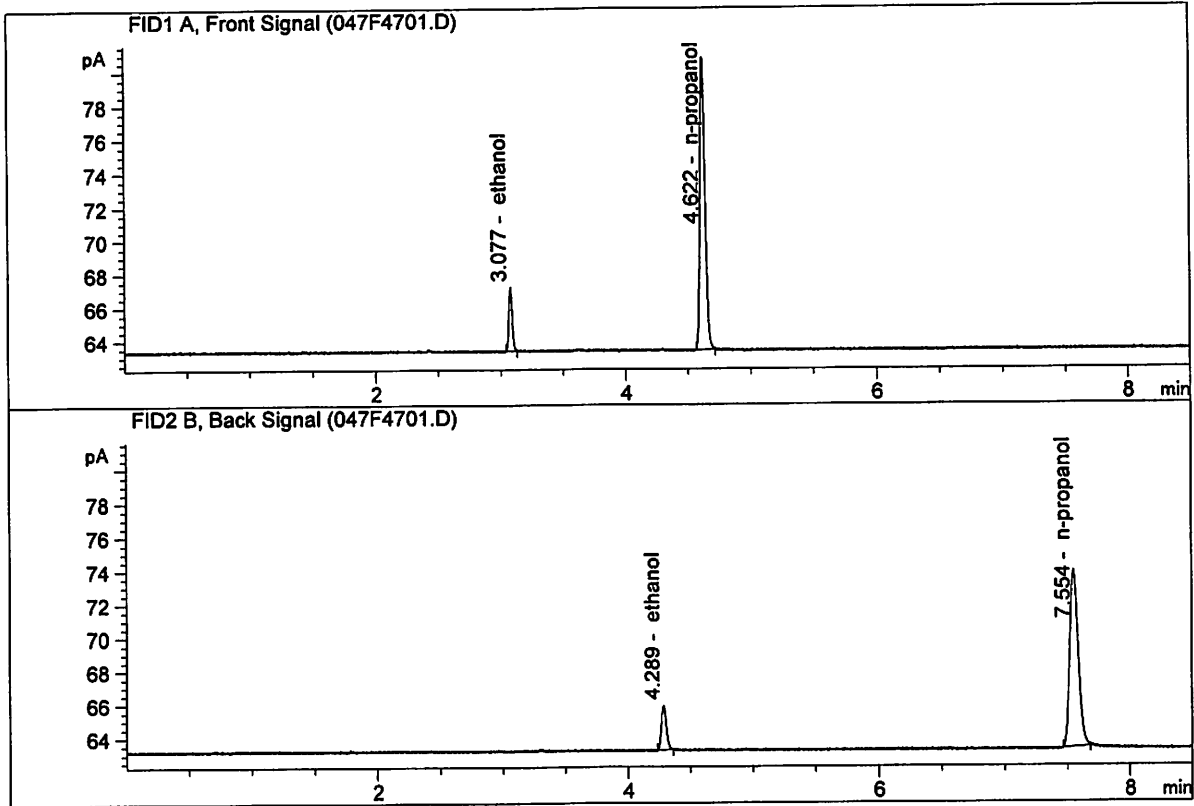


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.09112	0.0798	g/100cc
2.	Ethanol	Column 2:	7.15732	0.0803	g/100cc
3.	n-Propanol	Column 1:	49.28517	1.0000	g/100cc
4.	n-Propanol	Column 2:	50.26266	1.0000	g/100cc



ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-2-B  
 Laboratory : Meridian  
 Injection Date : Dec 19, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

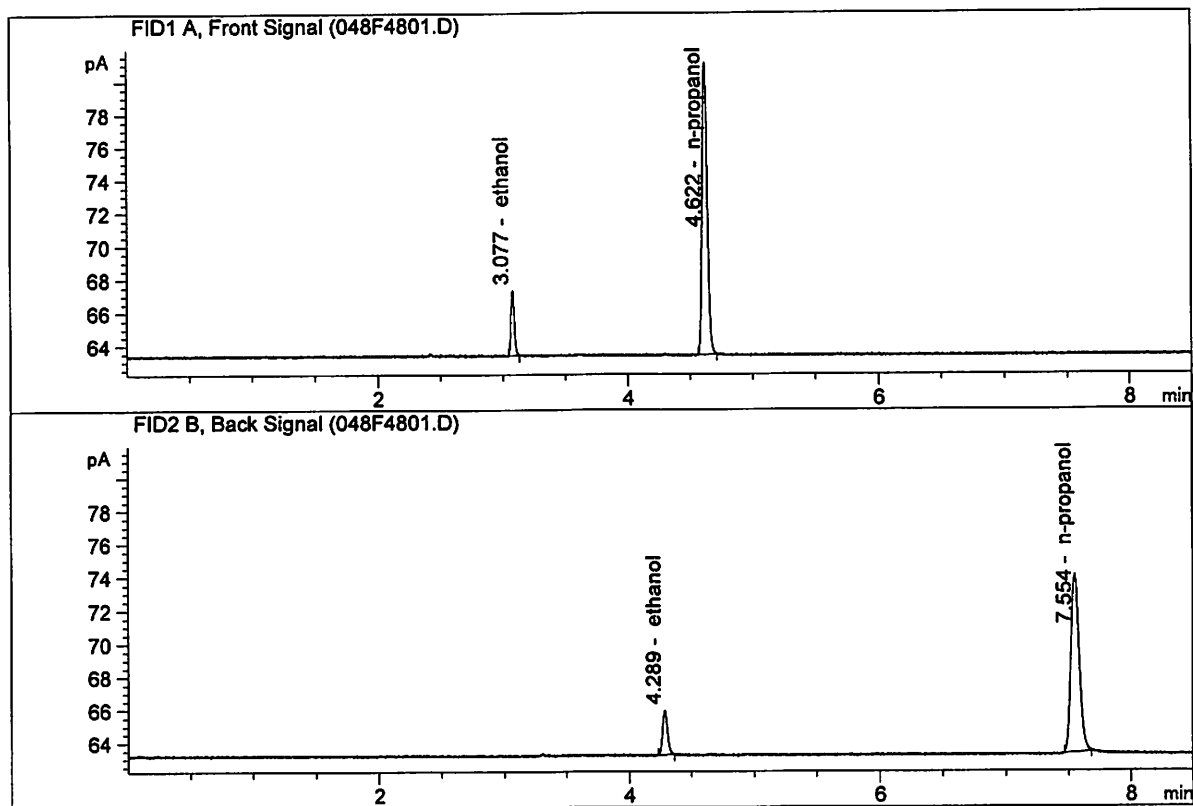

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.24414	0.0803	g/100cc
2.	Ethanol	Column 2:	7.31660	0.0809	g/100cc
3.	n-Propanol	Column 1:	50.00455	1.0000	g/100cc
4.	n-Propanol	Column 2:	50.99129	1.0000	g/100cc

# VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC2-2

Analysis Date(s): 20 Dec 2018

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean
Sample Results	0.2103	0.2104	0.0001	0.2103	0.2121
(g/100cc)	0.2140	0.2137	0.0003	0.2138	

**Analysis Method**

Refer to Blood Alcohol Method #1

**Instrument Information**

*Instrument method is stored centrally.*

Refer to Instrument Method: ALCOHOL.M  
Hamilton Auto-Dilutor Serial Number: ML600HC11378

**Reporting of Results**

**Uncertainty of Measurement (UM%): 5.00%**


Overall Mean (g/100cc)	Low	High	5% of Mean
0.212	0.201	0.223	0.011

	<b>Reported Result</b>  0.212
--	-------------------------------------

*Calibration and control data are stored centrally.*

ISP Forensic Services Blood Alcohol Report


Sample Name : QC2-2-A  
 Laboratory : Meridian  
 Injection Date : Dec 20, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

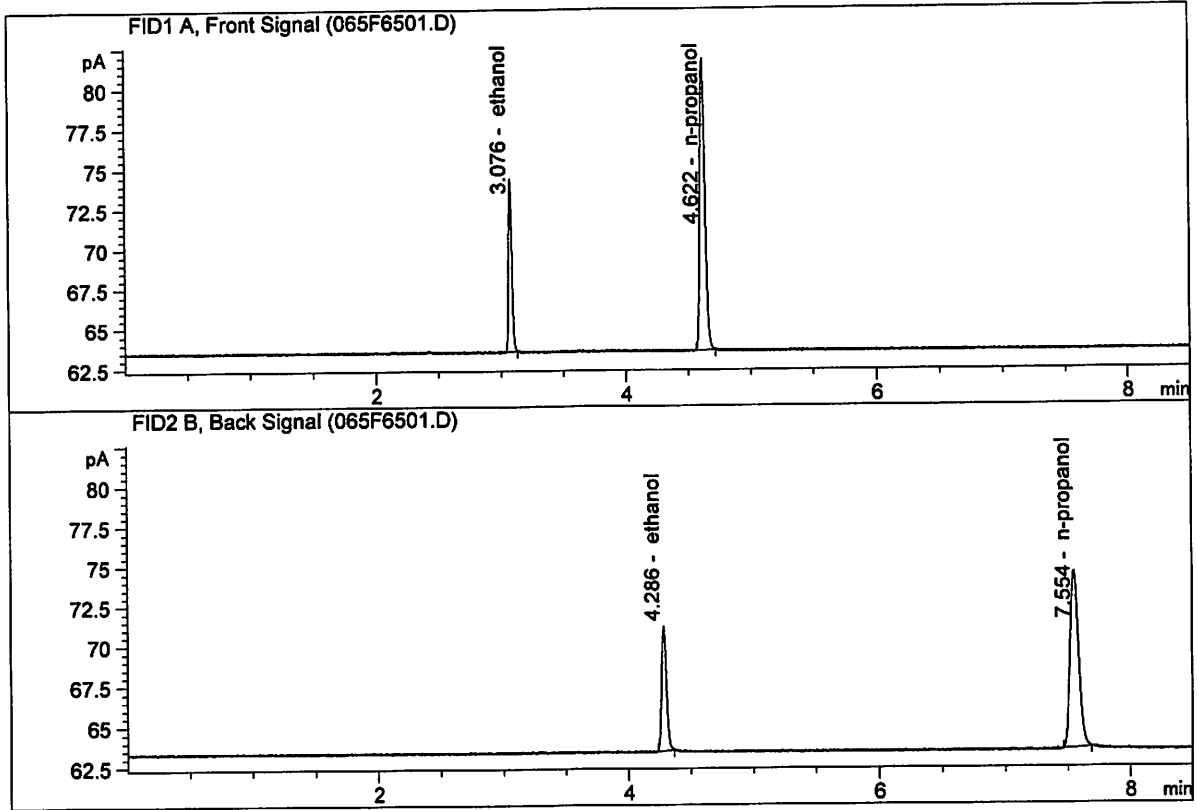

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	19.71055	0.2103	g/100cc
2.	Ethanol	Column 2:	20.43774	0.2104	g/100cc
3.	n-Propanol	Column 1:	51.44743	1.0000	g/100cc
4.	n-Propanol	Column 2:	52.53777	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report


Sample Name : QC2-2-B  
 Laboratory : Meridian  
 Injection Date : Dec 20, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

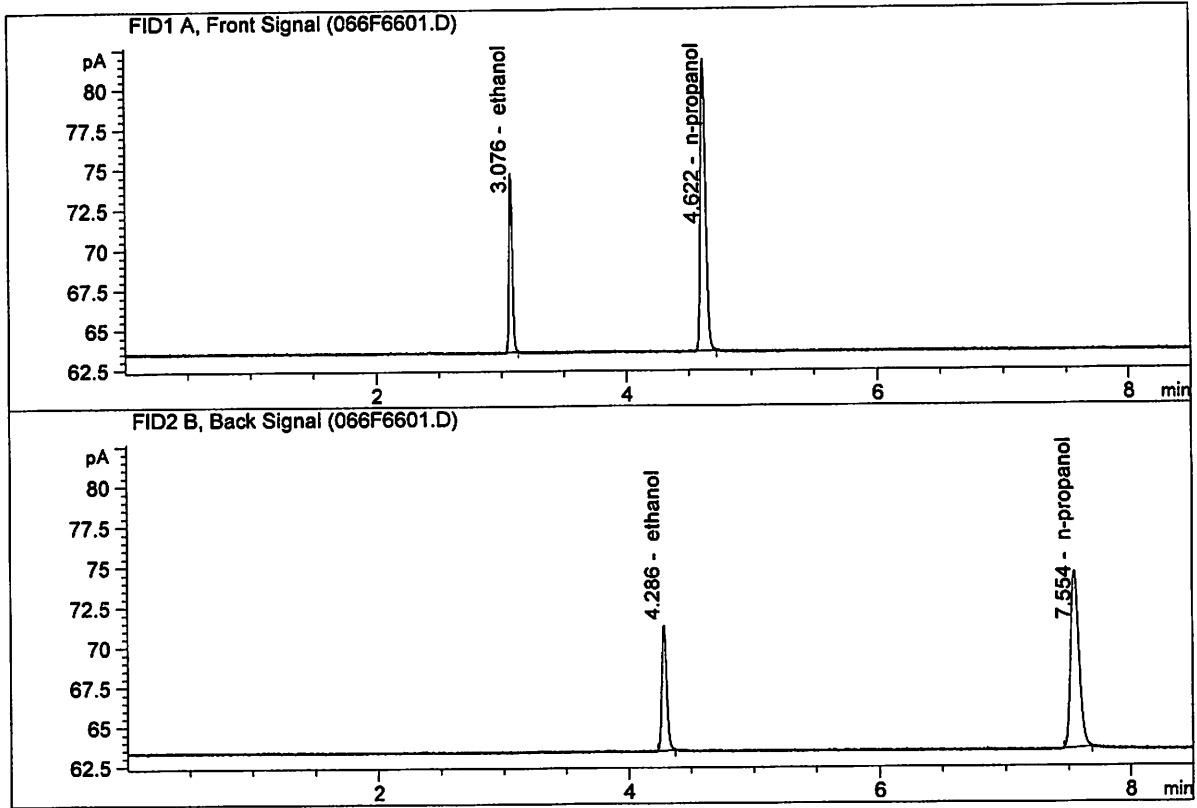

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	20.11096	0.2140	g/100cc
2.	Ethanol	Column 2:	20.88160	0.2137	g/100cc
3.	n-Propanol	Column 1:	51.57105	1.0000	g/100cc
4.	n-Propanol	Column 2:	52.81128	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report


Sample Name : BLK  
 Laboratory : Meridian  
 Injection Date : Dec 20, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

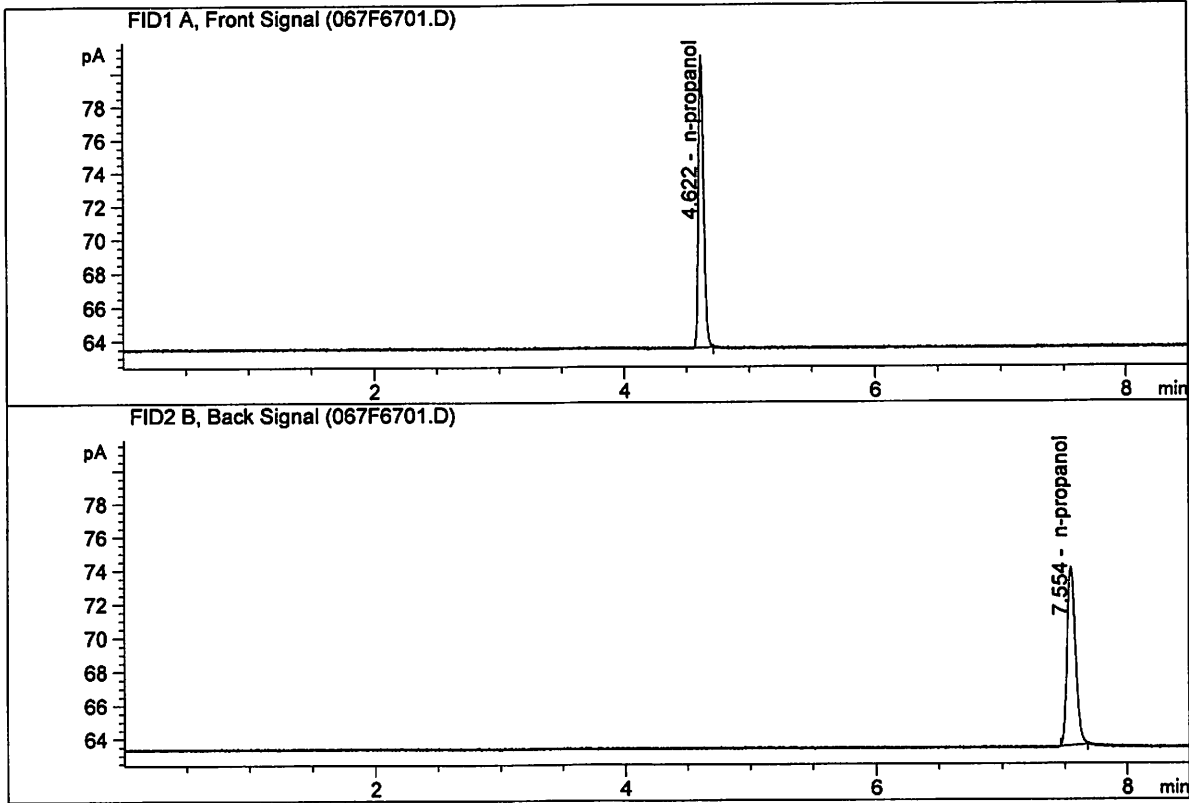

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	49.36553	1.0000	g/100cc
4.	n-Propanol	Column 2:	50.35127	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report


Sample Name : DFE 111914OM  
 Laboratory : Meridian  
 Injection Date : Dec 20, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

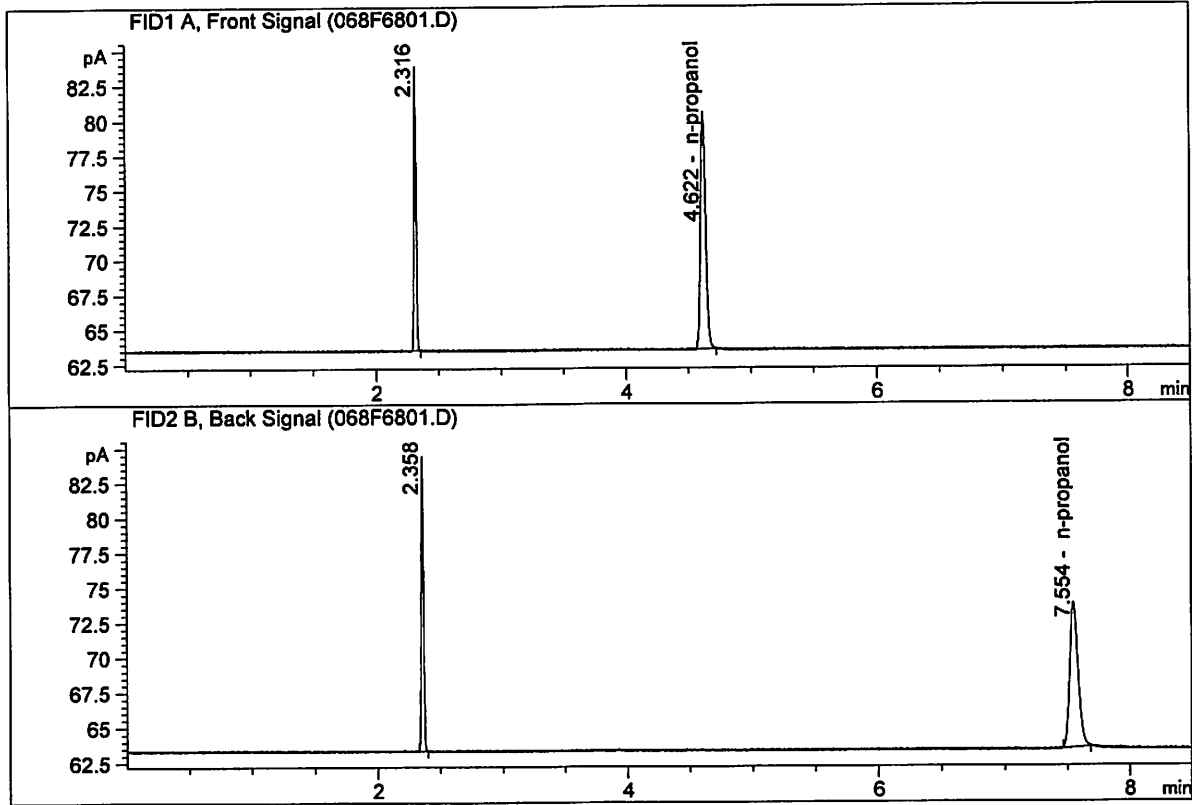

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	47.91829	1.0000	g/100cc
4.	n-Propanol	Column 2:	48.96500	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report


Sample Name : BLK  
 Laboratory : Meridian  
 Injection Date : Dec 20, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

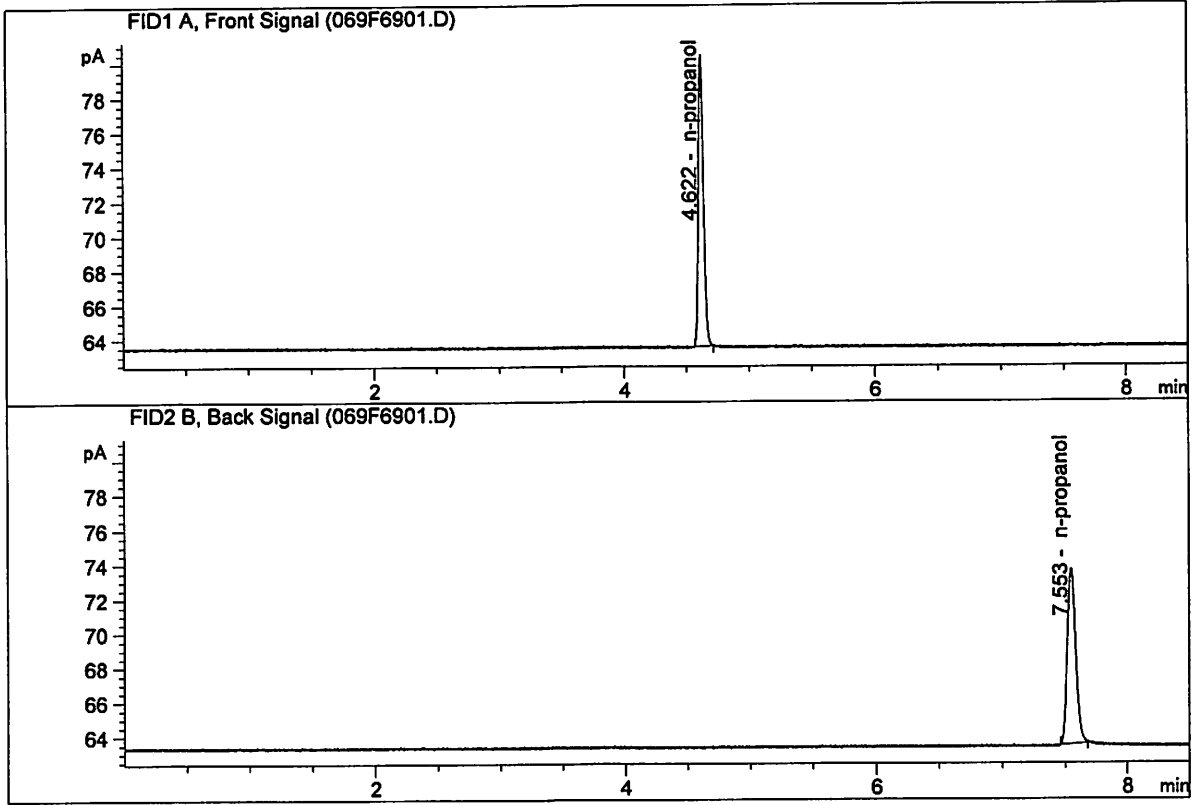

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	47.52639	1.0000	g/100cc
4.	n-Propanol	Column 2:	48.47232	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report

Sample Name : TFE 111914  
 Laboratory : Meridian  
 Injection Date : Dec 20, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

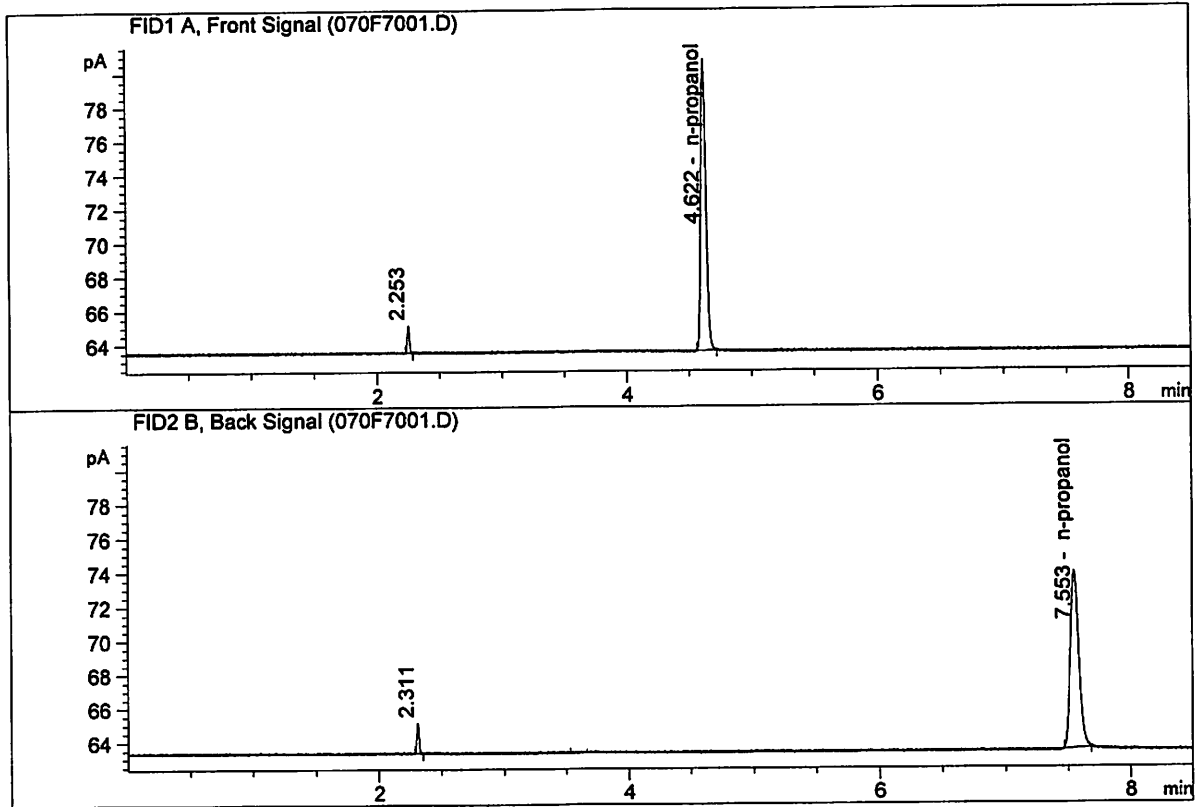


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	48.60394	1.0000	g/100cc
4.	n-Propanol	Column 2:	49.57930	1.0000	g/100cc



ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STD BLK  
 Laboratory : Meridian  
 Injection Date : Dec 20, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

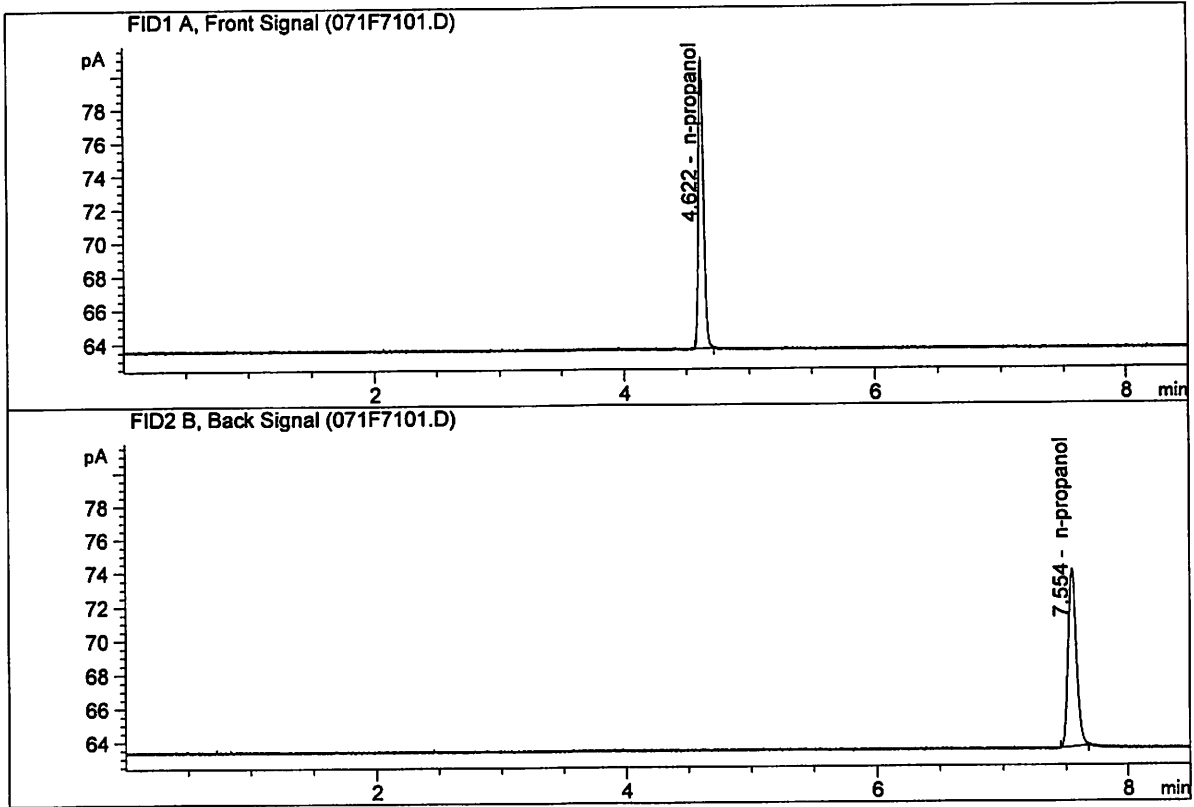

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	49.09373	1.0000	g/100cc
4.	n-Propanol	Column 2:	50.02436	1.0000	g/100cc

## S a m p l e S u m m a r y

Sequence table: C:\Chem32\1\Data\12-19-18\_SAMPLES\12-19-18\_SAMPLES 2018-12-19 15-10-28\12-19-18\_SAMPLES.S  
 Data directory path: C:\Chem32\1\Data\12-19-18\_SAMPLES\12-19-18\_SAMPLES 2018-12-19 15-10-28\  
 Logbook: C:\Chem32\1\Data\12-19-18\_SAMPLES\12-19-18\_SAMPLES 2018-12-19 15-10-28\12-19-18\_SAMPLES.LOG  
 Sequence start: 12/19/2018 3:25:20 PM  
 Sequence Operator: SYSTEM  
 Operator: SYSTEM

Method file name: C:\Chem32\1\Data\12-19-18\_SAMPLES\12-19-18\_SAMPLES 2018-12-19 15-10-28\  
 \ALCOHOL.M

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #	Cmp
1	1	1	INTERNAL STD BLK	-	1.0000	001F0101.D		2
2	2	1	MIX VOL FN060415	-	1.0000	002F0201.D		10
3	3	1	QC1-1-A	-	1.0000	003F0301.D		4
4	4	1	QC1-1-B	-	1.0000	004F0401.D		4
5	5	1	0.08 FN04171701-	-	1.0000	005F0501.D		4
6	6	1	0.08 FN04171701-	-	1.0000	006F0601.D		4
7	7	1	M2018-6049-2-A	-	1.0000	007F0701.D		2
8	8	1	M2018-6049-2-B	-	1.0000	008F0801.D		2
9	9	1	M2018-6057-1-A	-	1.0000	009F0901.D		6
10	10	1	M2018-6057-1-B	-	1.0000	010F1001.D		6
11	11	1	M2018-6071-1-A	-	1.0000	011F1101.D		4
12	12	1	M2018-6071-1-B	-	1.0000	012F1201.D		4
13	13	1	M2018-6072-1-A	-	1.0000	013F1301.D		4
14	14	1	M2018-6072-1-B	-	1.0000	014F1401.D		4
15	15	1	M2018-6073-1-A	-	1.0000	015F1501.D		4
16	16	1	M2018-6073-1-B	-	1.0000	016F1601.D		4
17	17	1	M2018-6074-1-A	-	1.0000	017F1701.D		4
18	18	1	M2018-6074-1-B	-	1.0000	018F1801.D		4
19	19	1	M2018-6092-1-A	-	1.0000	019F1901.D		4
20	20	1	M2018-6092-1-B	-	1.0000	020F2001.D		4
21	21	1	M2018-6110-1-A	-	1.0000	021F2101.D		4
22	22	1	M2018-6110-1-B	-	1.0000	022F2201.D		4
23	23	1	M2018-6111-1-A	-	1.0000	023F2301.D		4
24	24	1	M2018-6111-1-B	-	1.0000	024F2401.D		4
25	25	1	QC2-1-A	-	1.0000	025F2501.D		4
26	26	1	QC2-1-B	-	1.0000	026F2601.D		4
27	27	1	M2018-6112-1-A	-	1.0000	027F2701.D		4
28	28	1	M2018-6112-1-B	-	1.0000	028F2801.D		4
29	29	1	M2018-6113-1-A	-	1.0000	029F2901.D		4
30	30	1	M2018-6113-1-B	-	1.0000	030F3001.D		4
31	31	1	M2018-6128-1-A	-	1.0000	031F3101.D		4
32	32	1	M2018-6128-1-B	-	1.0000	032F3201.D		4
33	33	1	M2018-6129-1-A	-	1.0000	033F3301.D		4
34	34	1	M2018-6129-1-B	-	1.0000	034F3401.D		4
35	35	1	M2018-6130-1-A	-	1.0000	035F3501.D		6
36	36	1	M2018-6130-1-B	-	1.0000	036F3601.D		6
37	37	1	M2018-6134-1-A	-	1.0000	037F3701.D		4
38	38	1	M2018-6134-1-B	-	1.0000	038F3801.D		4
39	39	1	M2018-6140-1-A	-	1.0000	039F3901.D		4
40	40	1	M2018-6140-1-B	-	1.0000	040F4001.D		4
41	41	1	M2018-6143-1-A	-	1.0000	041F4101.D		4
42	42	1	M2018-6143-1-B	-	1.0000	042F4201.D		4
43	43	1	M2018-6156-1-A	-	1.0000	043F4301.D		4

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #	# Cmp
44	44	1	M2018-6156-1-B	-	1.0000	044F4401.D		4
45	45	1	M2018-6160-1-A	-	1.0000	045F4501.D		2
46	46	1	M2018-6160-1-B	-	1.0000	046F4601.D		2
47	47	1	QC1-2-A	-	1.0000	047F4701.D		4
48	48	1	QC1-2-B	-	1.0000	048F4801.D		4
49	49	1	M2018-6167-1-A	-	1.0000	049F4901.D		4
50	50	1	M2018-6167-1-B	-	1.0000	050F5001.D		4
51	51	1	M2018-6168-1-A	-	1.0000	051F5101.D		6
52	52	1	M2018-6168-1-B	-	1.0000	052F5201.D		6
53	53	1	M2018-6170-1-A	-	1.0000	053F5301.D		4
54	54	1	M2018-6170-1-B	-	1.0000	054F5401.D		4
55	55	1	M2018-6171-1-A	-	1.0000	055F5501.D		2
56	56	1	M2018-6171-1-B	-	1.0000	056F5601.D		2
57	57	1	M2018-6172-1-A	-	1.0000	057F5701.D		4
58	58	1	M2018-6172-1-B	-	1.0000	058F5801.D		4
59	59	1	P2018-3413-2-A	-	1.0000	059F5901.D		4
60	60	1	P2018-3413-2-B	-	1.0000	060F6001.D		4
61	61	1	P2018-3422-1-A	-	1.0000	061F6101.D		5
62	62	1	P2018-3422-1-B	-	1.0000	062F6201.D		4
63	63	1	P2018-3423-1-A	-	1.0000	063F6301.D		6
64	64	1	P2018-3423-1-B	-	1.0000	064F6401.D		6
65	65	1	QC2-2-A	-	1.0000	065F6501.D		4
66	66	1	QC2-2-B	-	1.0000	066F6601.D		4
67	67	1	BLK	-	1.0000	067F6701.D		2
68	68	1	DFE 111914OM	-	1.0000	068F6801.D		2
69	69	1	BLK	-	1.0000	069F6901.D		2
70	70	1	TFE 111914	-	1.0000	070F7001.D		2
71	71	1	INTERNAL STD BLK	-	1.0000	071F7101.D		2


Method file name: C:\Chem32\1\Data\12-19-18\_SAMPLES\12-19-18\_SAMPLES 2018-12-19 15-10-28  
 \SHUTDOWN.M

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #	# Cmp
72	72	1	EMPTY	-	1.0000	072F7201.D		0

dg

ISP Forensic Services Blood Alcohol Report


Sample Name : 0.050 FN06231406  
 Laboratory : Meridian  
 Injection Date : Dec 11, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

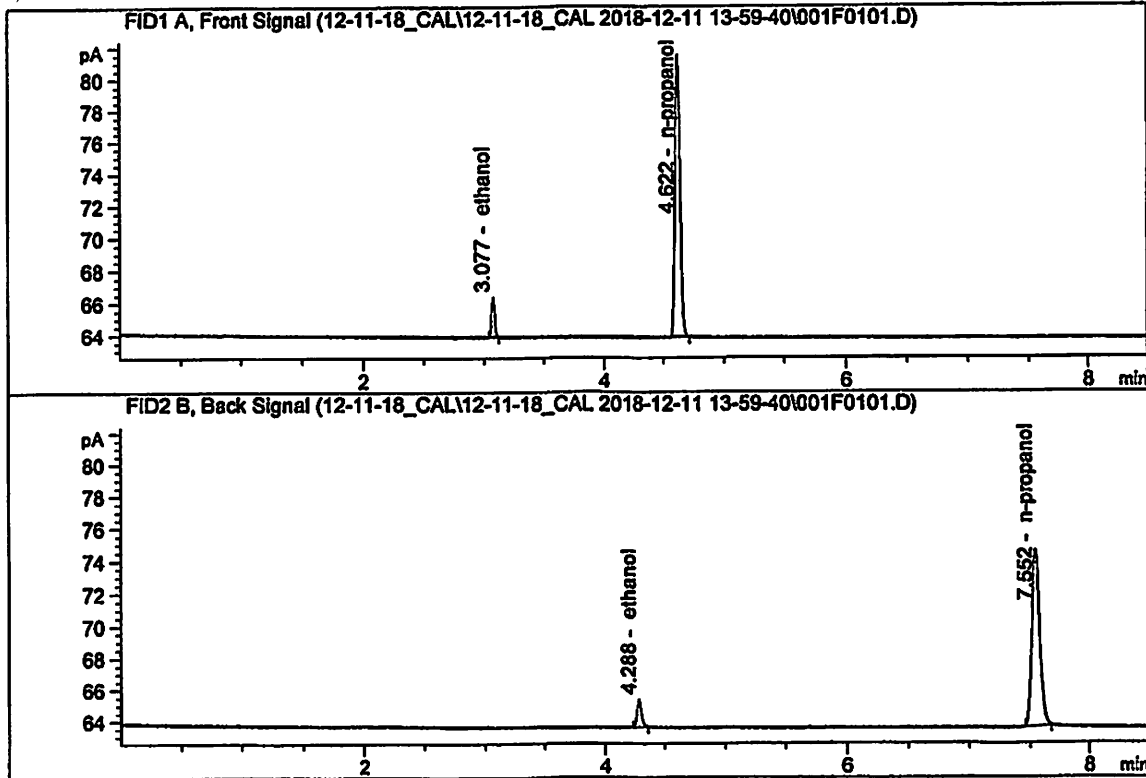

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	4.51683	0.0505	g/100cc
2.	Ethanol	Column 2:	4.66970	0.0520	g/100cc
3.	n-Propanol	Column 1:	50.11460	1.0000	g/100cc
4.	n-Propanol	Column 2:	52.56495	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report


Sample Name : 0.100 FN08101601  
 Laboratory : Meridian  
 Injection Date : Dec 11, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

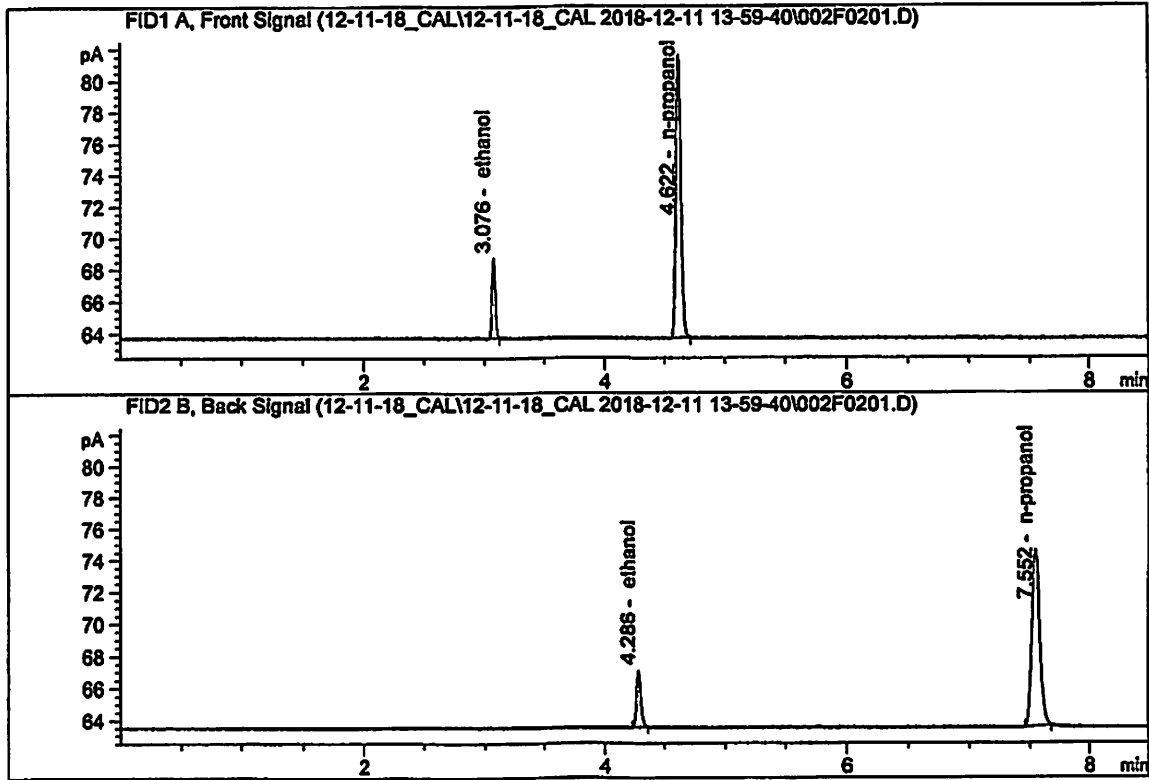

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	9.16088	0.0998	g/100cc
2.	Ethanol	Column 2:	9.51851	0.1003	g/100cc
3.	n-Propanol	Column 1:	50.70458	1.0000	g/100cc
4.	n-Propanol	Column 2:	52.77800	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report


Sample Name : 0.200 FN12011401  
 Laboratory : Meridian  
 Injection Date : Dec 11, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

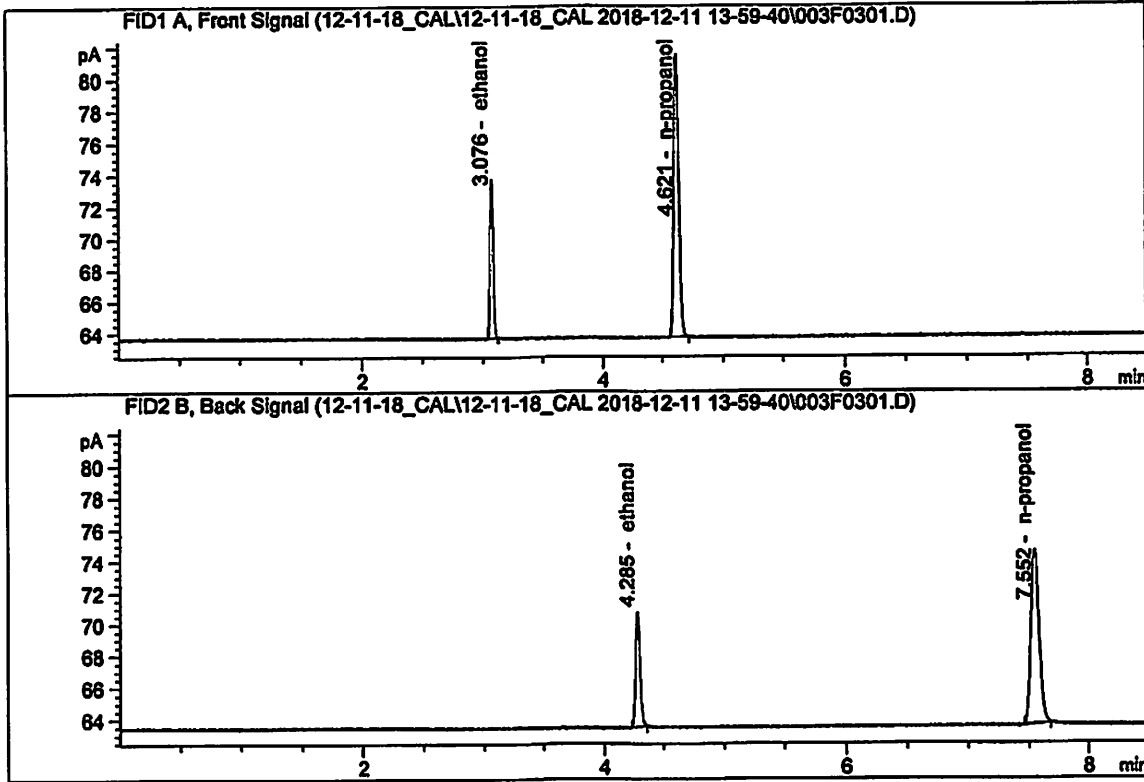

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	18.38613	0.1997	g/100cc
2.	Ethanol	Column 2:	19.14837	0.1976	g/100cc
3.	n-Propanol	Column 1:	50.54507	1.0000	g/100cc
4.	n-Propanol	Column 2:	52.49086	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report


Sample Name : 0.300 FN02121601  
 Laboratory : Meridian  
 Injection Date : Dec 11, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

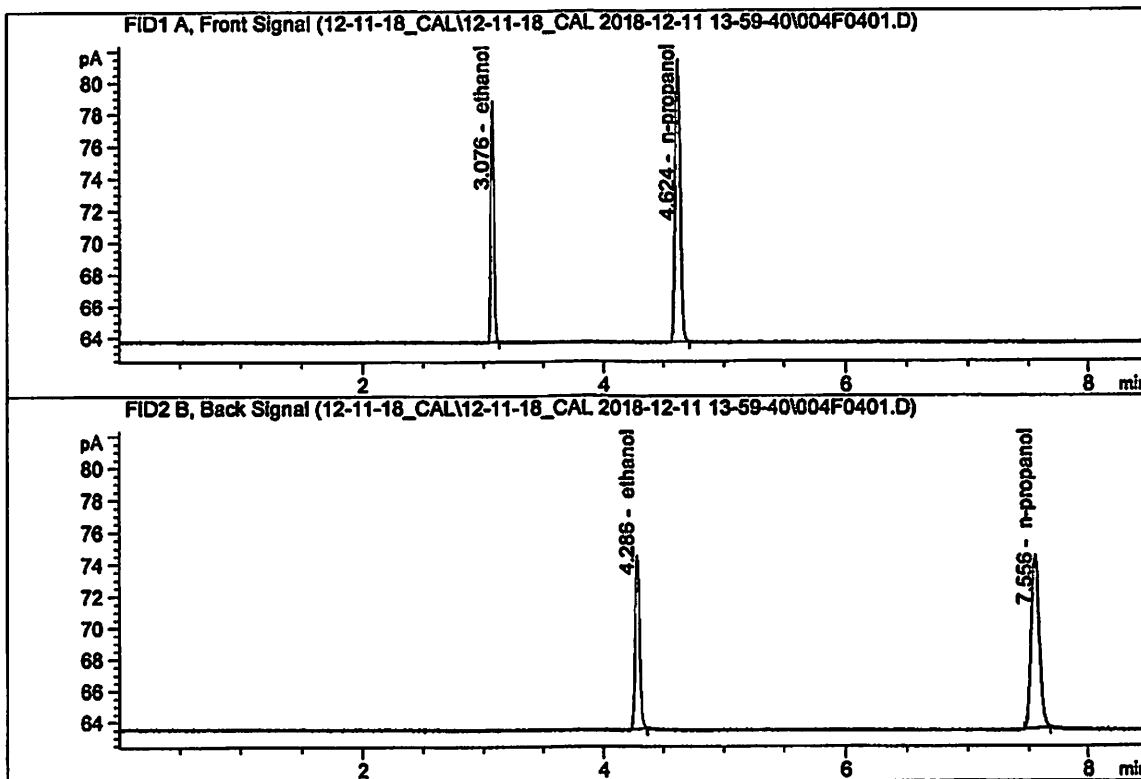

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	27.62826	0.2997	g/100cc
2.	Ethanol	Column 2:	29.04338	0.2984	g/100cc
3.	n-Propanol	Column 1:	50.49660	1.0000	g/100cc
4.	n-Propanol	Column 2:	52.24192	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.500 FN08031602  
 Laboratory : Meridian  
 Injection Date : Dec 11, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

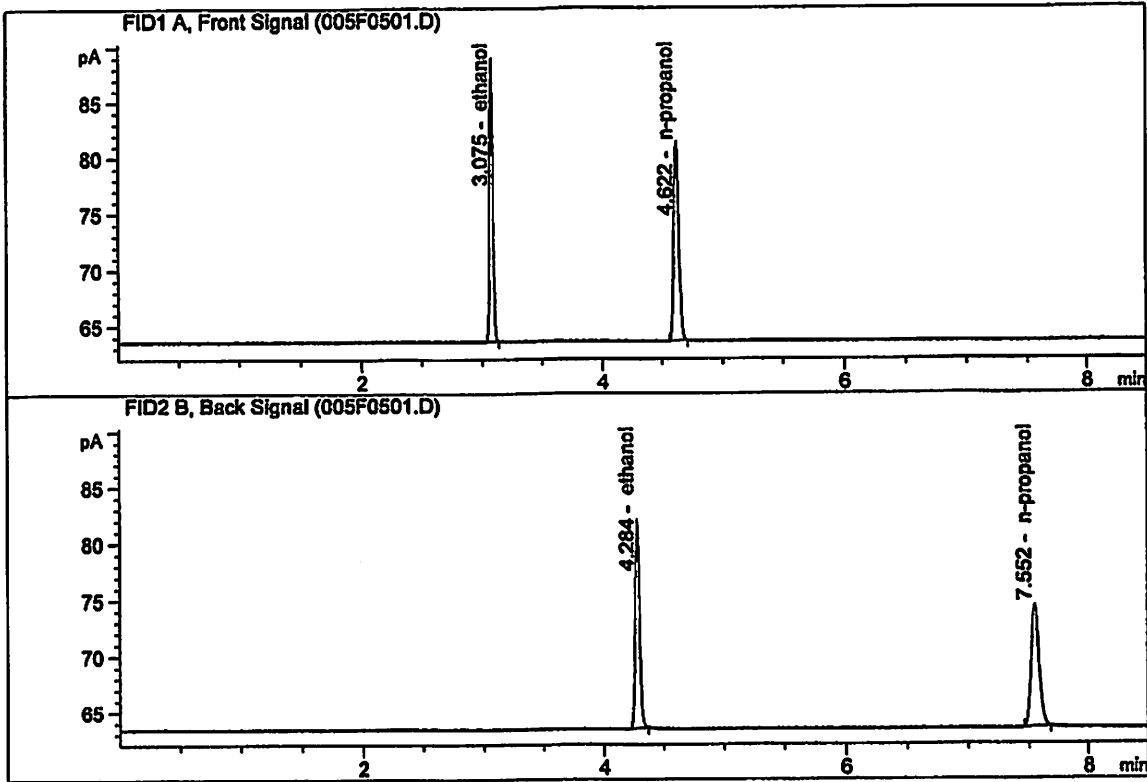


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	46.18552	0.5003	g/100cc
2.	Ethanol	Column 2:	49.01530	0.5016	g/100cc
3.	n-Propanol	Column 1:	50.48219	1.0000	g/100cc
4.	n-Propanol	Column 2:	52.07859	1.0000	g/100cc



ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STANDARD BLANK  
 Laboratory : Meridian  
 Injection Date : Dec 11, 2018  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

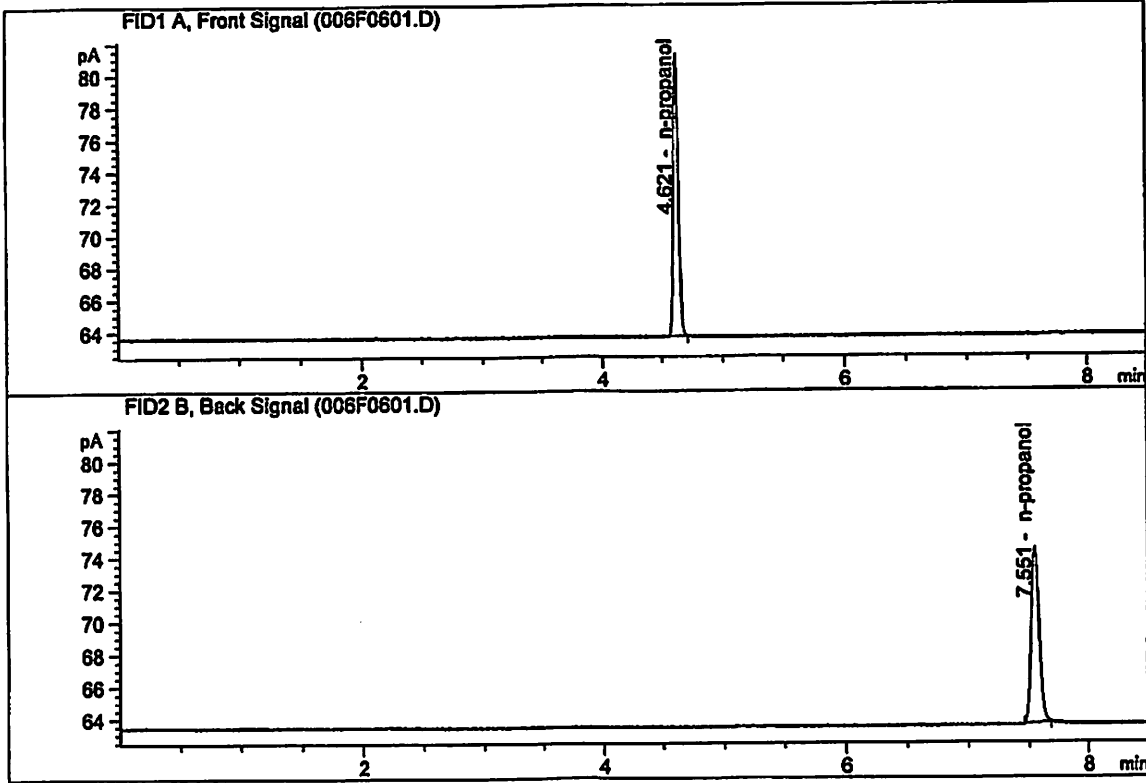

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	49.96477	1.0000	g/100cc
4.	n-Propanol	Column 2:	51.62820	1.0000	g/100cc

S a m p l e S u m m a r y

Sequence table: C:\Chem32\1\Data\12-11-18\_CAL\12-11-18\_CAL 2018-12-11 13-59-40\12-11-18\_CAL.S  
 Data directory path: C:\Chem32\1\Data\12-11-18\_CAL\12-11-18\_CAL 2018-12-11 13-59-40\  
 Logbook: C:\Chem32\1\Data\12-11-18\_CAL\12-11-18\_CAL 2018-12-11 13-59-40\12-11-18\_CAL.LOG  
 Sequence start: 12/11/2018 2:14:18 PM  
 Sequence Operator: SYSTEM  
 Operator: SYSTEM  
 Method file name: C:\Chem32\1\Data\12-11-18\_CAL\12-11-18\_CAL 2018-12-11 13-59-40\ALCOHOL.M

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #	Cmp
1	1	1	0.050 FN06231406	-	1.0000	001F0101.D	*	4
2	2	1	0.100 FN08101601	-	1.0000	002F0201.D	*	4
3	3	1	0.200 FN12011401	-	1.0000	003F0301.D	*	4
4	4	1	0.300 FN02121601	-	1.0000	004F0401.D	*	4
5	5	1	0.500 FN08031602	-	1.0000	005F0501.D	*	4
6	6	1	INTERNAL STANDAR	-	1.0000	006F0601.D		2

JC

=====  
Calibration Table  
=====

-----  
General Calibration Setting  
-----

Calib. Data Modified : Tuesday, December 11, 2018 3:04:51 PM  
Signals calculated separately : No

Rel. Reference Window : 0.000 %  
Abs. Reference Window : 0.100 min  
Rel. Non-ref. Window : 0.000 %  
Abs. Non-ref. Window : 0.100 min  
Uncalibrated Peaks : not reported  
Partial Calibration : Yes, identified peaks are recalibrated  
Correct All Ret. Times: No, only for identified peaks

Curve Type : Linear  
Origin : Ignored  
Weight : Equal

Recalibration Settings:  
Average Response : Average all calibrations  
Average Retention Time: Floating Average New 75%

Calibration Report Options :  
Printout of recalibrations within a sequence:  
Calibration Table after Recalibration  
Normal Report after Recalibration  
If the sequence is done with bracketing:  
Results of first cycle (ending previous bracket)

Default Sample ISTD Information (if not set in sample table):

ISTD #	ISTD Amount [g/100cc]	Name
1	1.00000	n-propanol
2	1.00000	n-propanol

-----  
Signal Details  
-----

Signal 1: FID1 A, Front Signal  
Signal 2: FID2 B, Back Signal  
-----

-----  
Overview Table  
-----

JC

RT	Sig	Lvl	Amount [g/100cc]	Area	Rsp.Factor	Ref	ISTD #	Compound
2.586	1	1	1.00000	3.69669	2.70512e-1	No	No 1	methanol
2.809	1	1	1.00000	4.26100	2.34687e-1	No	No 2	Acetaldehyde
2.977	2	1	1.00000	4.26100	2.34687e-1	No	No 2	Acetaldehyde
3.075	1	1	5.00000e-2	4.51683	1.10697e-2	No	No 1	ethanol
		2	1.00000e-1	9.16088	1.09160e-2			
		3	2.00000e-1	18.38613	1.08778e-2			
		4	3.00000e-1	27.62826	1.08584e-2			
		5	5.00000e-1	46.18552	1.08259e-2			
3.388	2	1	1.00000	4.26062	2.34707e-1	No	No 2	methanol
3.628	1	1	1.00000	9.73055	1.02769e-1	No	No 1	isopropyl alcohol
4.285	2	1	5.00000e-2	4.66970	1.07073e-2	No	No 2	ethanol
		2	1.00000e-1	9.51851	1.05058e-2			
		3	2.00000e-1	19.14837	1.04448e-2			
		4	3.00000e-1	29.04338	1.03294e-2			
		5	5.00000e-1	49.01530	1.02009e-2			
4.308	1	1	1.00000	6.49940	1.53860e-1	No	No 1	acetone
4.620	1	1	1.00000	50.11460	1.99543e-2	No	Yes 1	n-propanol
		2	1.00000	50.70458	1.97221e-2			
		3	1.00000	50.54507	1.97843e-2			
		4	1.00000	50.49660	1.98033e-2			
		5	1.00000	50.48219	1.98090e-2			
4.661	2	1	1.00000	6.89301	1.45075e-1	No	No 2	acetone
4.969	2	1	1.00000	10.70642	9.34019e-2	No	No 2	isopropyl alcohol
7.550	2	1	1.00000	52.56495	1.90241e-2	No	Yes 2	n-propanol
		2	1.00000	52.77800	1.89473e-2			
		3	1.00000	52.49086	1.90509e-2			
		4	1.00000	52.24192	1.91417e-2			
		5	1.00000	52.07859	1.92017e-2			

Peak Sum Table


\*\*\*No Entries in table\*\*\*

61 Warnings or Errors (10 first messages follow) :


- Warning : Curve requires more calibration points., (methanol)
- Warning : Curve requires more calibration points. at 2.586 min, signal 1
- Warning : Curve requires more calibration points. at 2.809 min, signal 1
- Warning : Curve requires more calibration points. at 2.977 min, signal 2
- Warning : Curve requires more calibration points. at 3.388 min, signal 2
- Warning : Curve requires more calibration points. at 3.628 min, signal 1
- Warning : Curve requires more calibration points. at 4.308 min, signal 1
- Warning : Curve requires more calibration points. at 4.62 min, signal 1
- Warning : Curve requires more calibration points. at 4.661 min, signal 2
- Warning : Curve requires more calibration points. at 4.969 min, signal 2

JG


=====  
 Calibration Curves  
 =====

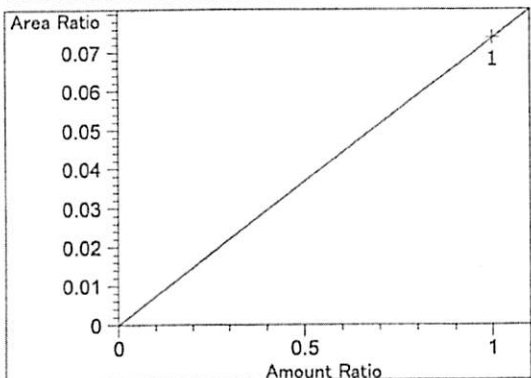


methanol at exp. RT: 2.586  
 FID1 A, Front Signal  
 Correlation: 1.00000  
 Residual Std. Dev.: 0.00000  
 Formula:  $y = mx + b$   
 m: 7.37648e-2  
 b: 0.00000  
 x: Amount Ratio  
 y: Area Ratio

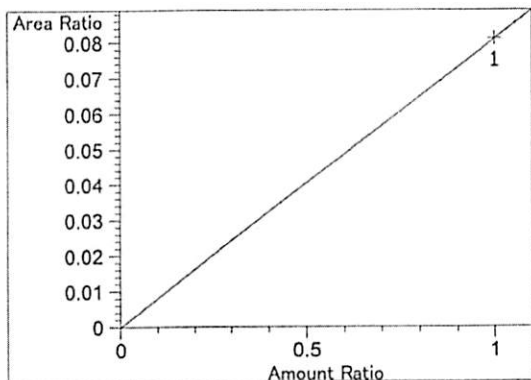

Acetaldehyde at exp. RT: 2.809  
 FID1 A, Front Signal  
 Correlation: 1.00000  
 Residual Std. Dev.: 0.00000  
 Formula:  $y = mx + b$   
 m: 8.10616e-2  
 b: 0.00000  
 x: Amount Ratio  
 y: Area Ratio

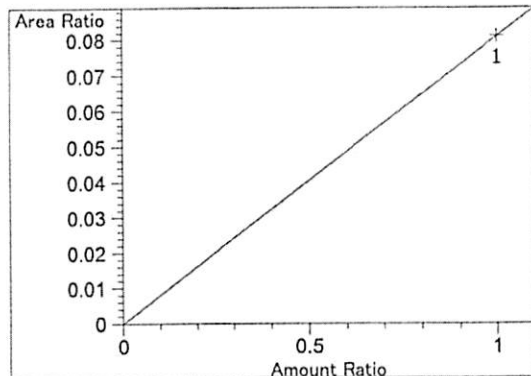


Acetaldehyde at exp. RT: 2.977  
 FID2 B, Back Signal  
 Correlation: 1.00000  
 Residual Std. Dev.: 0.00000  
 Formula:  $y = mx + b$   
 m: 8.10616e-2  
 b: 0.00000  
 x: Amount Ratio  
 y: Area Ratio

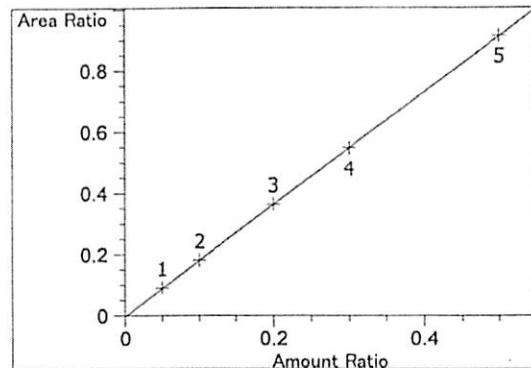


ethanol at exp. RT: 3.075  
 FID1 A, Front Signal  
 Correlation: 1.00000  
 Residual Std. Dev.: 0.00074  
 Formula:  $y = mx + b$   
 m: 1.83356  
 b: -2.40276e-3  
 x: Amount Ratio  
 y: Area Ratio


JK

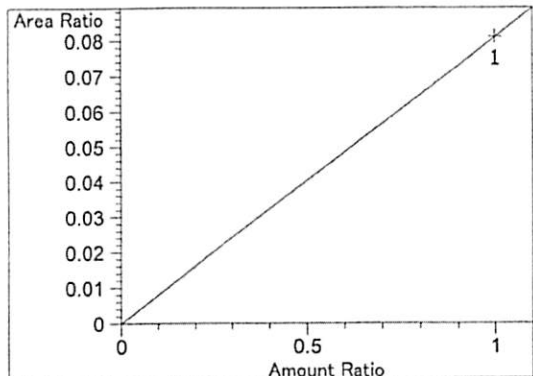


methanol at exp. RT: 3.388  
 FID2 B, Back Signal  
 Correlation: 1.00000  
 Residual Std. Dev.: 0.00000  
 Formula:  $y = mx + b$   
 m: 8.10545e-2  
 b: 0.00000  
 x: Amount Ratio  
 y: Area Ratio

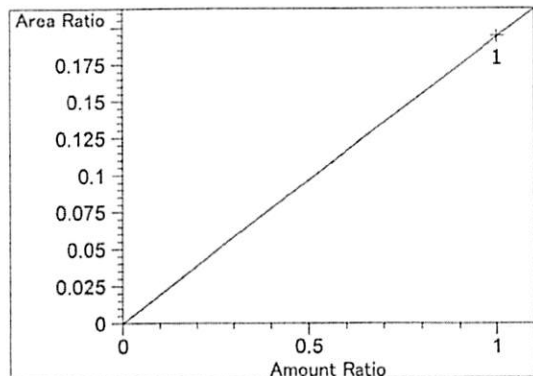


isopropyl alcohol at exp. RT: 3.628  
 FID1 A, Front Signal  
 Correlation: 1.00000  
 Residual Std. Dev.: 0.00000  
 Formula:  $y = mx + b$   
 m: 1.94166e-1  
 b: 0.00000  
 x: Amount Ratio  
 y: Area Ratio

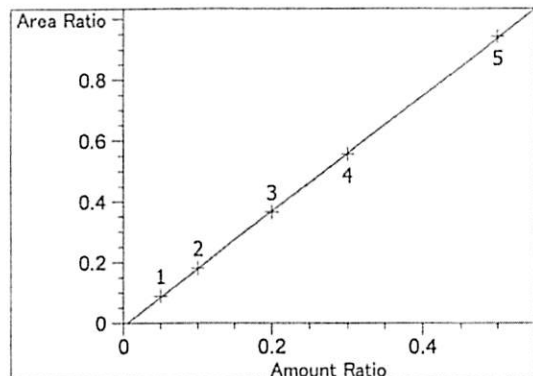


ethanol at exp. RT: 4.285  
 FID2 B, Back Signal  
 Correlation: 0.99994  
 Residual Std. Dev.: 0.00426  
 Formula:  $y = mx + b$   
 m: 1.89574  
 b: -9.79940e-3  
 x: Amount Ratio  
 y: Area Ratio

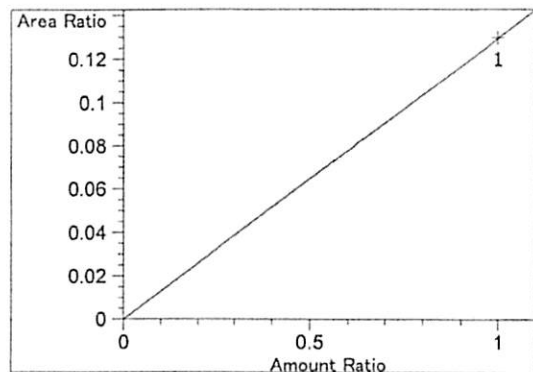


acetone at exp. RT: 4.308  
 FID1 A, Front Signal  
 Correlation: 1.00000  
 Residual Std. Dev.: 0.00000  
 Formula:  $y = mx + b$   
 m: 1.29691e-1  
 b: 0.00000  
 x: Amount Ratio  
 y: Area Ratio

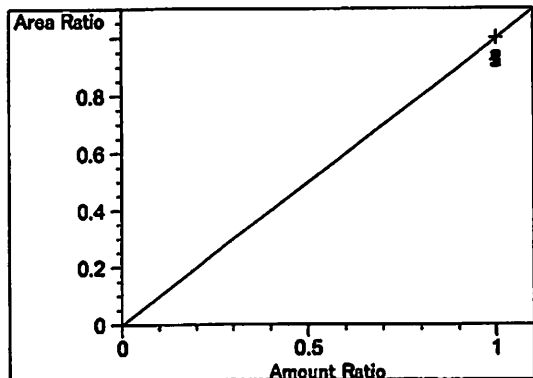


n-propanol at exp. RT: 4.620  
FID1 A, Front Signal  
Correlation: 1.00000  
Residual Std. Dev.: 0.00000  
Formula:  $y = mx + b$   
m: 1.00000  
b: 0.00000  
x: Amount Ratio  
y: Area Ratio

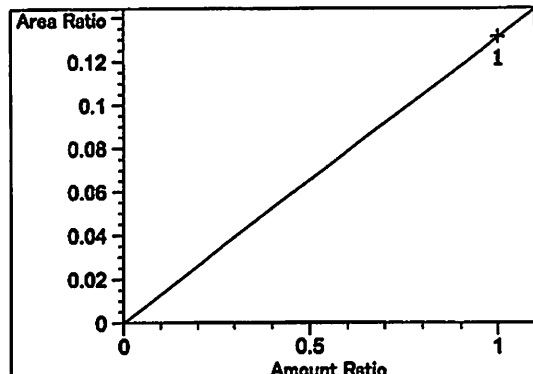

acetone at exp. RT: 4.661  
FID2 B, Back Signal  
Correlation: 1.00000  
Residual Std. Dev.: 0.00000  
Formula:  $y = mx + b$   
m: 1.31133e-1  
b: 0.00000  
x: Amount Ratio  
y: Area Ratio

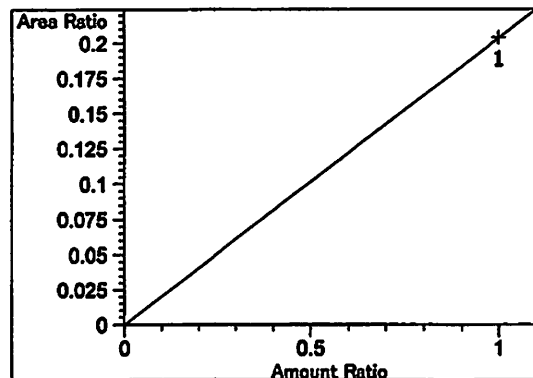

isopropyl alcohol at exp. RT: 4.969  
FID2 B, Back Signal  
Correlation: 1.00000  
Residual Std. Dev.: 0.00000  
Formula:  $y = mx + b$   
m: 2.03680e-1  
b: 0.00000  
x: Amount Ratio  
y: Area Ratio

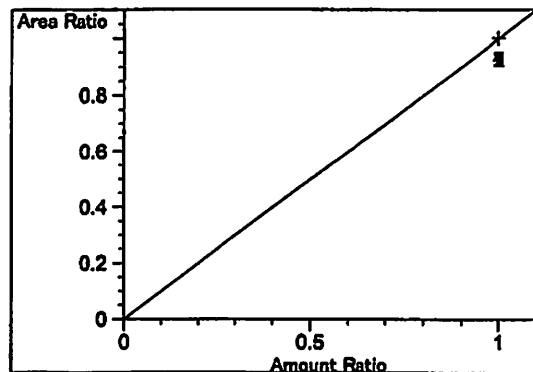

n-propanol at exp. RT: 7.550  
FID2 B, Back Signal  
Correlation: 1.00000  
Residual Std. Dev.: 0.00000  
Formula:  $y = mx + b$   
m: 1.00000  
b: 0.00000  
x: Amount Ratio  
y: Area Ratio

=====

JK