

Quantitative Analysis for Ethanol & Qualitative Analysis for Other Volatiles

Analytical Method(s): 1.0

Device: Hamilton MICROLAB 600A Liquid Processor/Dilutor Serial Number: ML600HC11378

Volatiles Quality Assurance Controls Run Date(s): 3/1/19

Calibration Date: 2/20/19

Control level	Expiration	Lot #	Target Value	Acceptable Range	Overall Results
Level 1	Jan-22	1801036	0.0812	0.0731-0.0893	0.0785 g/100cc
					0.0816 g/100cc
Level 2	Mar-22	1803028	0.2035	0.1832-0.2238	0.2048 g/100cc
					g/100cc
Multi-Component mixture:					
Curve Fit:		Column 1	Lot #	FN06041502	ok
			0.99998	Column2	0.99996

Ethanol Calibration Reference Material						
Calibrator level	Target Value	Acceptable Range	Column 1	Column 2	Precision	Mean
50	0.050	0.045 - 0.055	0.0502	0.0520	0.0018	0.0511
100	0.100	0.090 - 0.110	0.0991	0.0998	0.0007	0.0994
200	0.200	0.180 - 0.220	0.1999	0.1978	0.0021	0.1988
300	0.300	0.270 - 0.330	0.3016	0.2992	0.0024	0.3004
500	0.500	0.450 - 0.550	0.4992	0.5012	0.002	0.5002

Aqueous Controls			
Control level	Target Value	Acceptable Range	Overall Results
80	0.080	0.076 - 0.084	0.080 g/100cc




Revision: 1

Issue Date: 01/03/2019

Issuing Authority: Quality Manager

Worklist: 3000


<u>LAB CASE</u>	<u>ITEM</u>	<u>TASK ID</u>	<u>DESCRIPTION</u>
M2019-0877	1	142113	Alcohol Analysis
M2019-0878	2	142115	Alcohol Analysis
M2019-0890	3	143299	Alcohol Analysis
M2019-0906	1	142256	Alcohol Analysis
M2019-0910	1	142269	Alcohol Analysis
M2019-0938	1	142501	Alcohol Analysis
M2019-0962	1	142593	Alcohol Analysis
M2019-0978	1	142746	Alcohol Analysis
M2019-0979	1	142747	Alcohol Analysis
M2019-0980	1	142748	Alcohol Analysis
M2019-1017	1	142891	Alcohol Analysis
M2019-1031	1	143036	Alcohol Analysis
M2019-1042	1	143076	Alcohol Analysis
M2019-1043	1	143078	Alcohol Analysis
M2019-1064	1	143153	Alcohol Analysis

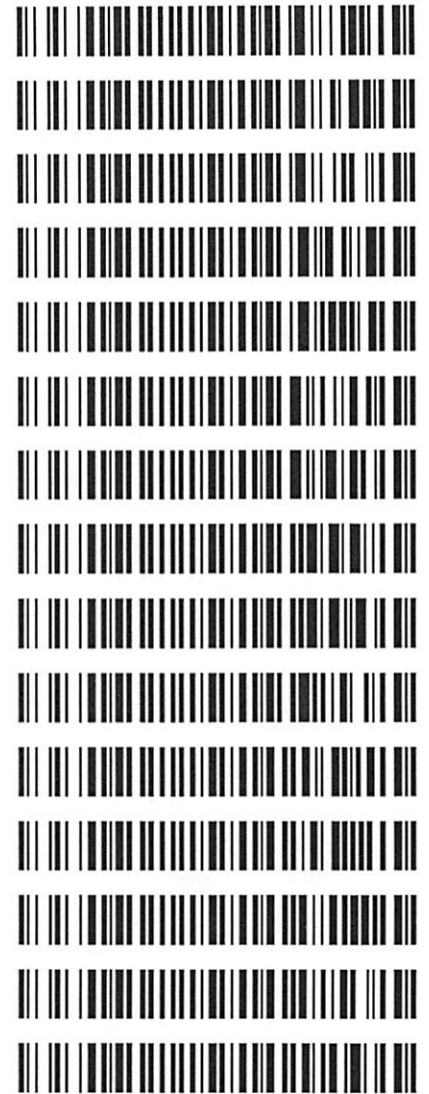

JL

ISP Forensic Services Blood Alcohol Report


Sample Name : INTERNAL STD BLK 1
 Laboratory : Meridian
 Injection Date : Mar 1, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

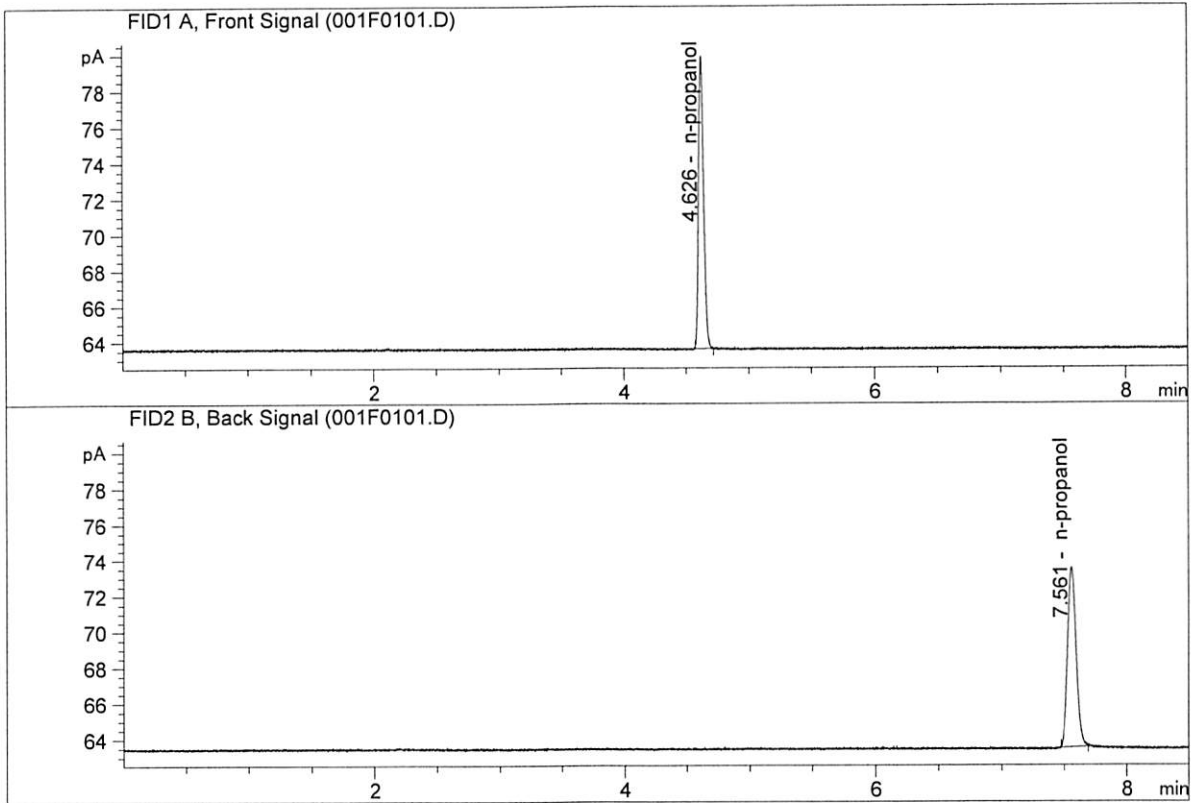

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	46.15866	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.92090	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report

Sample Name : MIX VOL FN06041502
 Laboratory : Meridian
 Injection Date : Mar 1, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

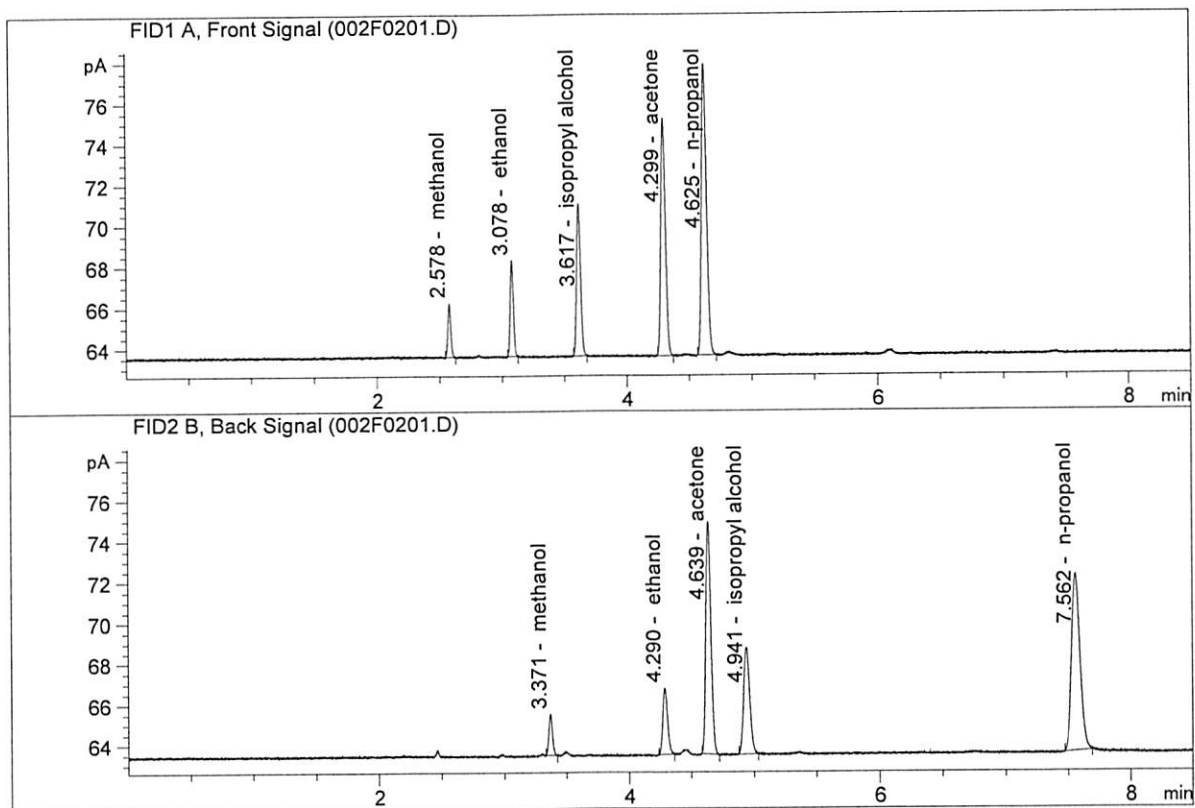

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	8.47593	0.1059	g/100cc
2.	Ethanol	Column 2:	8.68036	0.1058	g/100cc
3.	n-Propanol	Column 1:	40.29431	1.0000	g/100cc
4.	n-Propanol	Column 2:	41.39556	1.0000	g/100cc

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC1-1

Analysis Date(s): 01 Mar 2019

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.0786	0.0789	0.0003	0.0787	0.0785	
(g/100cc)	0.0775	0.0793	0.0018	0.0784		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: Alcohol.m
Hamilton Auto-Dilutor Serial Number: ML600HC11378

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.078	0.074	0.082	0.004

	Reported Result	
	0.078	

Calibration and control data are stored centrally.

JG


Revision: 1

Issue Date: 01/04/2019

Issuing Authority: Quality Manager

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-1-A
 Laboratory : Meridian
 Injection Date : Mar 1, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

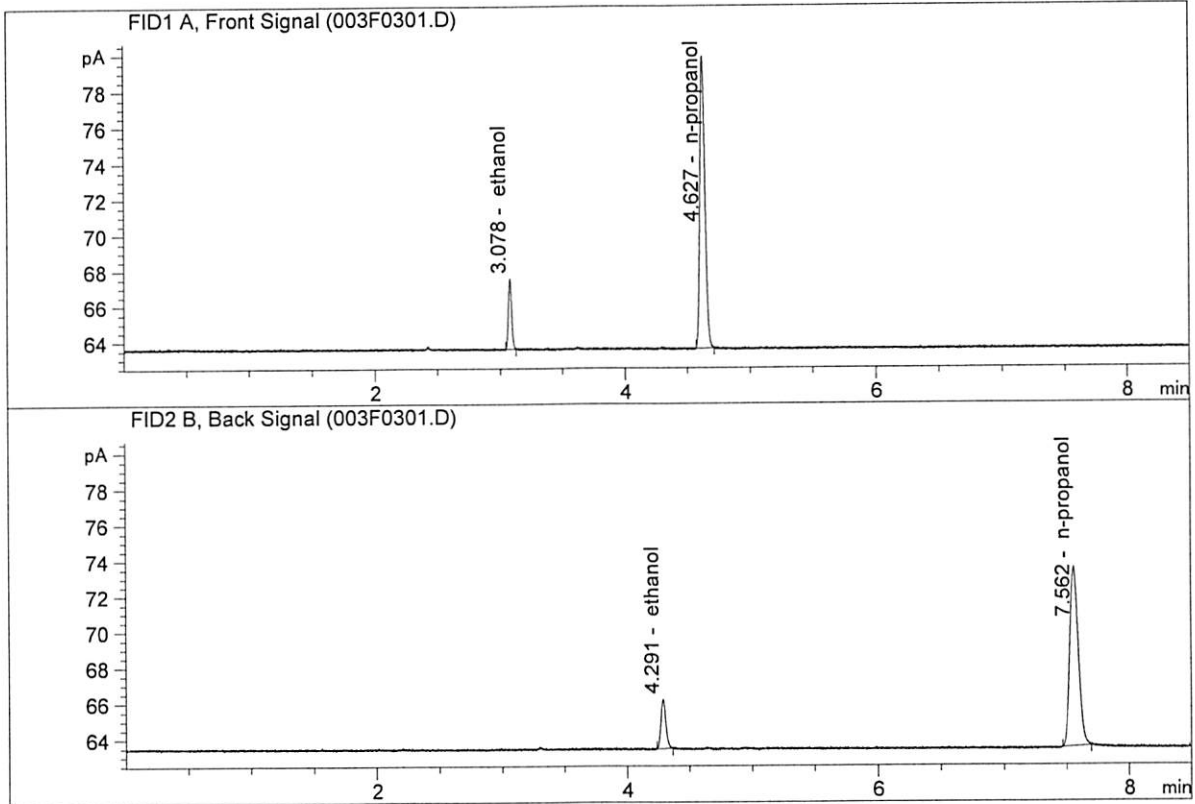


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.21237	0.0786	g/100cc
2.	Ethanol	Column 2:	7.37155	0.0789	g/100cc
3.	n-Propanol	Column 1:	46.24708	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.81854	1.0000	g/100cc

JL

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-1-B
 Laboratory : Meridian
 Injection Date : Mar 1, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

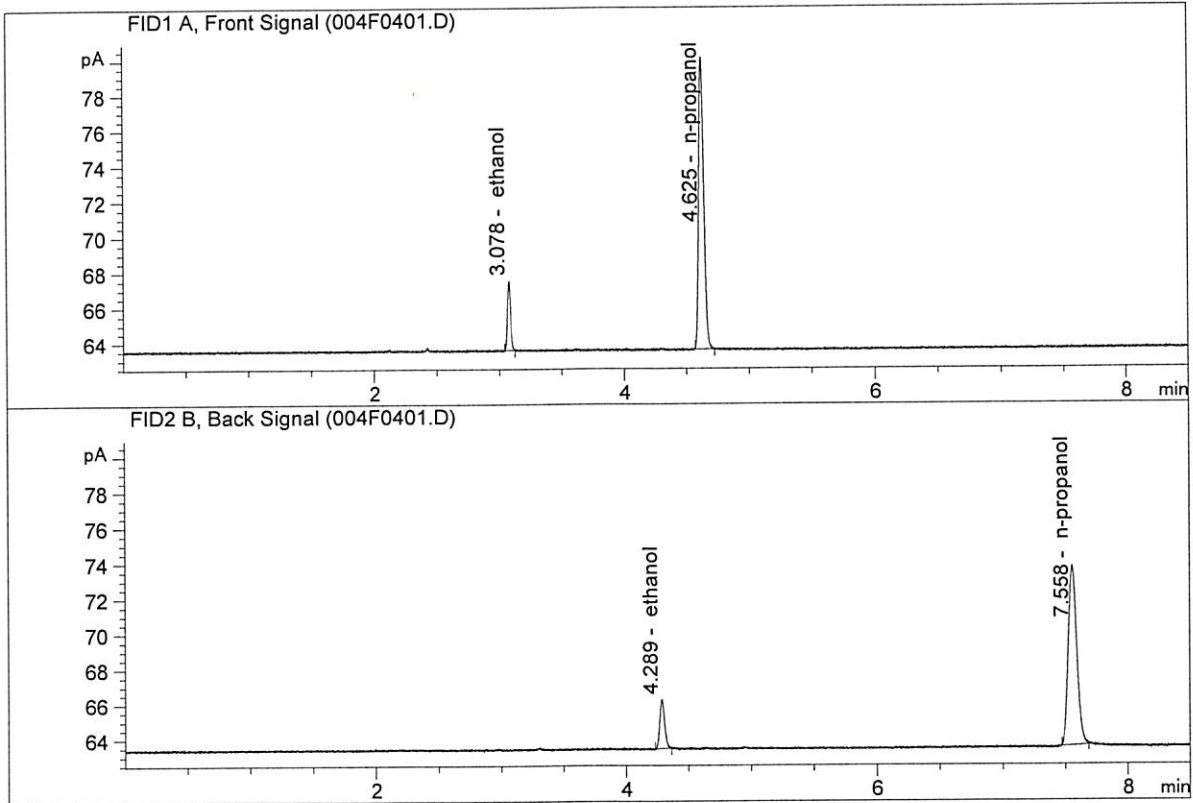

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.24346	0.0775	g/100cc
2.	Ethanol	Column 2:	7.49732	0.0793	g/100cc
3.	n-Propanol	Column 1:	47.08802	1.0000	g/100cc
4.	n-Propanol	Column 2:	48.40458	1.0000	g/100cc

JG

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: 0.08 FN04171701

Analysis Date(s): 01 Mar 2019

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.0798	0.0801	0.0003	0.0799	0.0801	
(g/100cc)	0.0800	0.0806	0.0006	0.0803		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: Alcohol.m
Hamilton Auto-Dilutor Serial Number: ML600HC11378

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.080	0.076	0.084	0.004

	Reported Result	
	0.080	

Calibration and control data are stored centrally.

56


Revision: 1

Issue Date: 01/04/2019

Issuing Authority: Quality Manager

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.08 FN04171701-A
 Laboratory : Meridian
 Injection Date : Mar 1, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014 -CN11041167

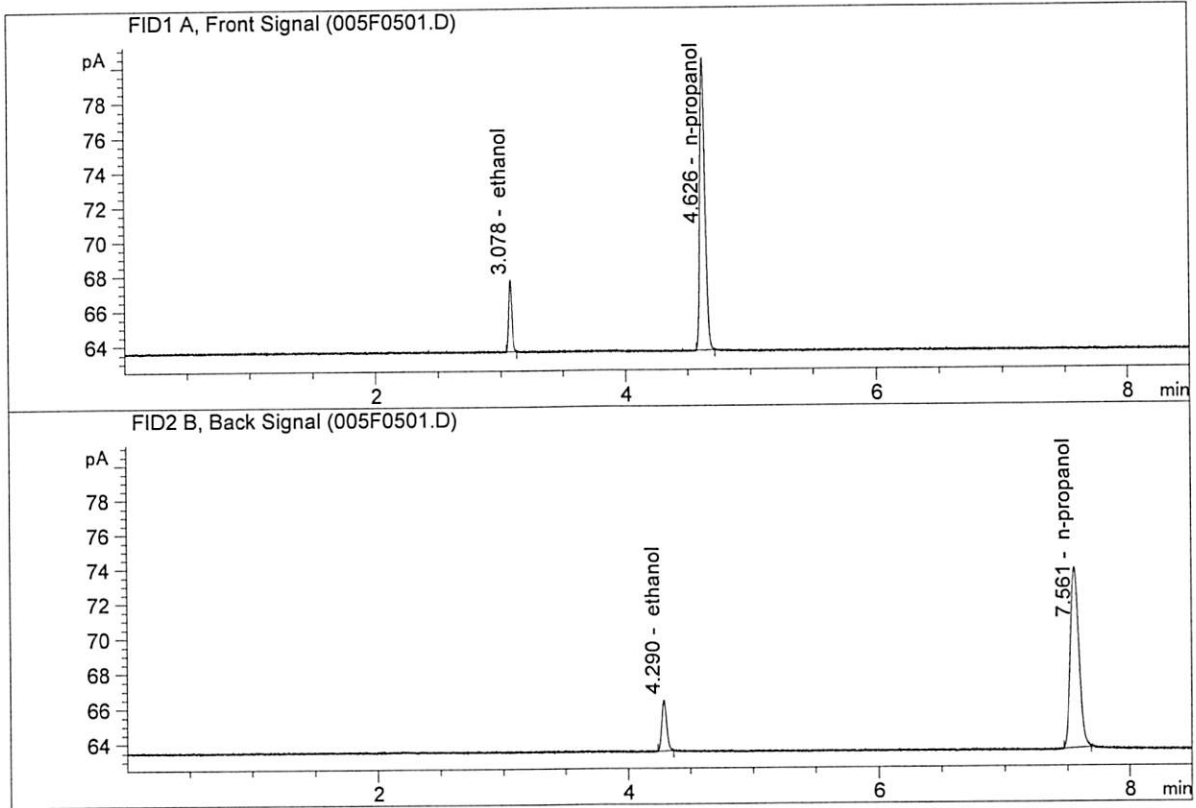


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.55293	0.0798	g/100cc
2.	Ethanol	Column 2:	7.71935	0.0801	g/100cc
3.	n-Propanol	Column 1:	47.68484	1.0000	g/100cc
4.	n-Propanol	Column 2:	49.30645	1.0000	g/100cc

JG

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.08 FN04171701-B
 Laboratory : Meridian
 Injection Date : Mar 1, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

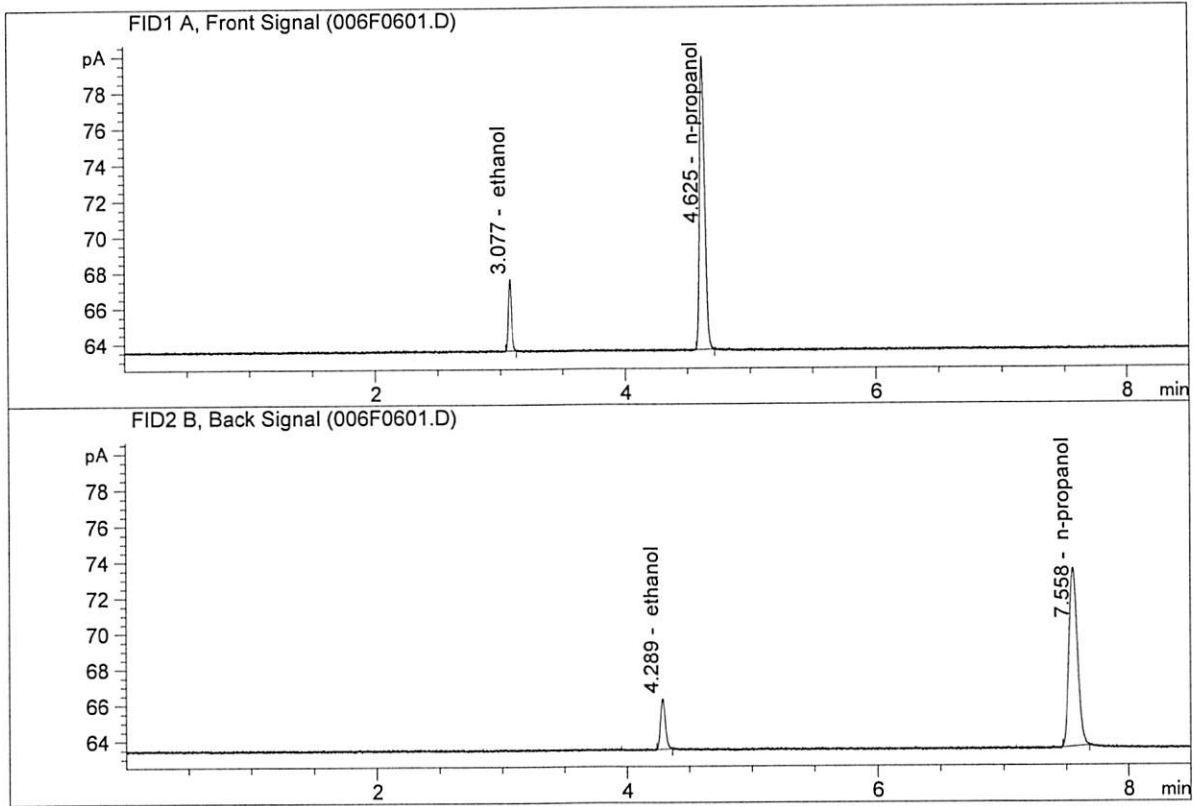

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.34074	0.0800	g/100cc
2.	Ethanol	Column 2:	7.48703	0.0806	g/100cc
3.	n-Propanol	Column 1:	46.25636	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.50018	1.0000	g/100cc

JK

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC2-1

Analysis Date(s): 01 Mar 2019

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.2049	0.2036	0.0013	0.2042	0.2048	
(g/100cc)	0.2054	0.2055	0.0001	0.2054		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: Alcohol.m
Hamilton Auto-Dilutor Serial Number: ML600HC11378

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.204	0.193	0.215	0.011

	Reported Result	
	0.204	

Calibration and control data are stored centrally.

JL


Revision: 1

Issue Date: 01/04/2019

Issuing Authority: Quality Manager

ISP Forensic Services Blood Alcohol Report

Sample Name : QC2-1-A
 Laboratory : Meridian
 Injection Date : Mar 1, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

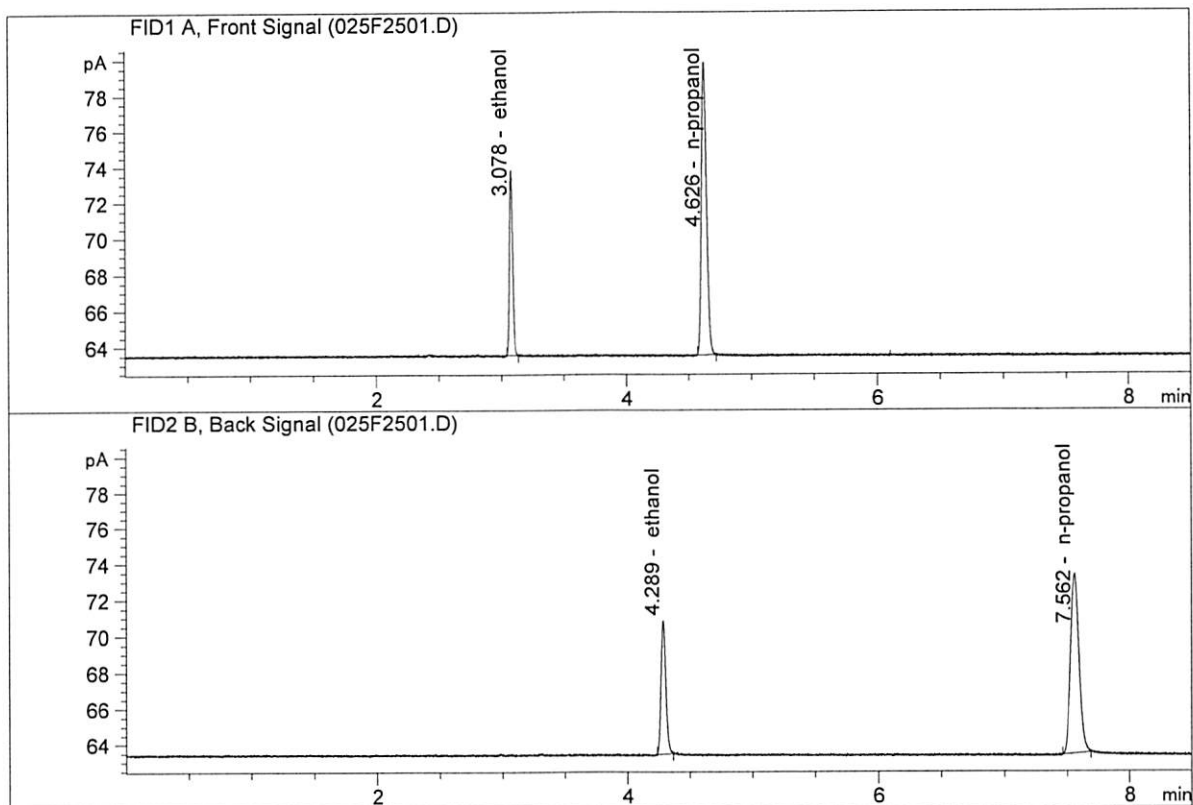


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	18.81201	0.2049	g/100cc
2.	Ethanol	Column 2:	19.52403	0.2036	g/100cc
3.	n-Propanol	Column 1:	46.15205	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.40908	1.0000	g/100cc

JG

ISP Forensic Services Blood Alcohol Report

Sample Name : QC2-1-B
 Laboratory : Meridian
 Injection Date : Mar 1, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

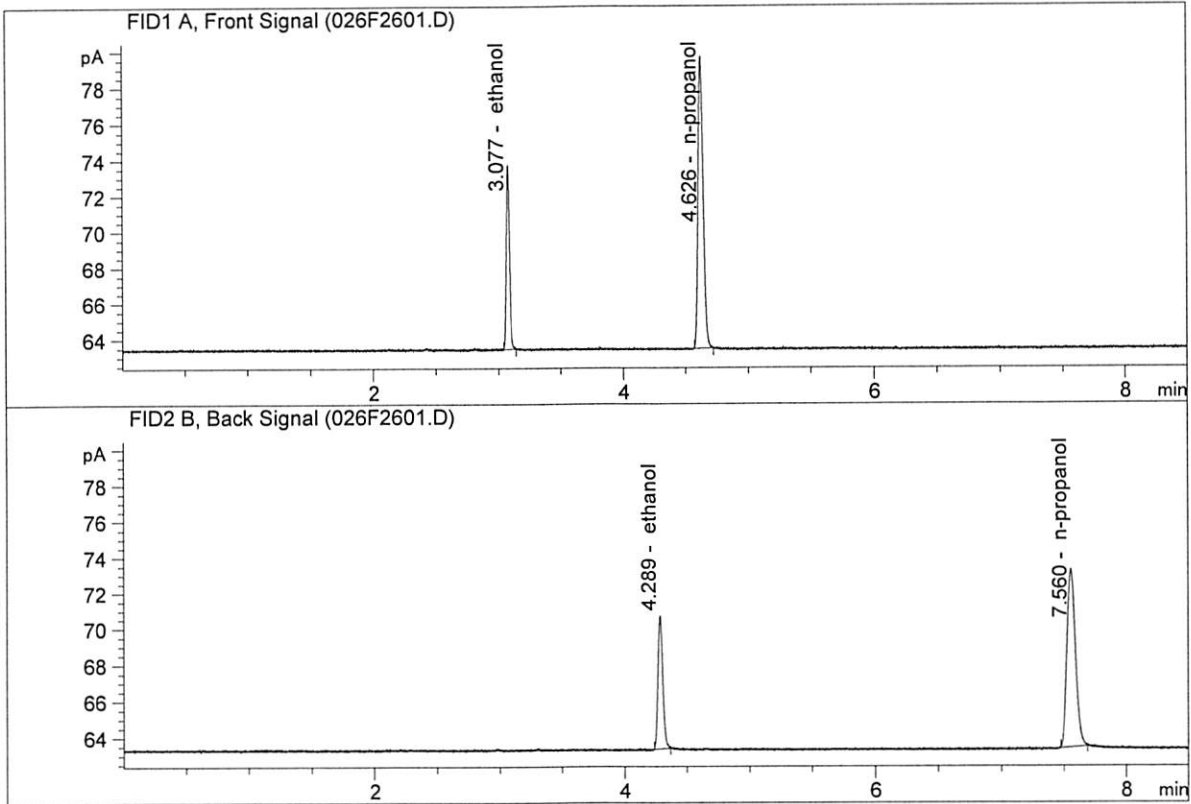

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	18.78131	0.2054	g/100cc
2.	Ethanol	Column 2:	19.51062	0.2055	g/100cc
3.	n-Propanol	Column 1:	45.95141	1.0000	g/100cc
4.	n-Propanol	Column 2:	46.92561	1.0000	g/100cc

JK

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC1-2

Analysis Date(s): 01 Mar 2019

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean
Sample Results	0.0814	0.0829	0.0015	0.0821	0.0816
(g/100cc)	0.0807	0.0817	0.0010	0.0812	

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: Alcohol.m
Hamilton Auto-Dilutor Serial Number: ML600HC11378

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.081	0.076	0.086	0.005

Reported Result	
0.081	

Calibration and control data are stored centrally.

JL


Revision: 1

Issue Date: 01/04/2019

Issuing Authority: Quality Manager

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-2-A
 Laboratory : Meridian
 Injection Date : Mar 1, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

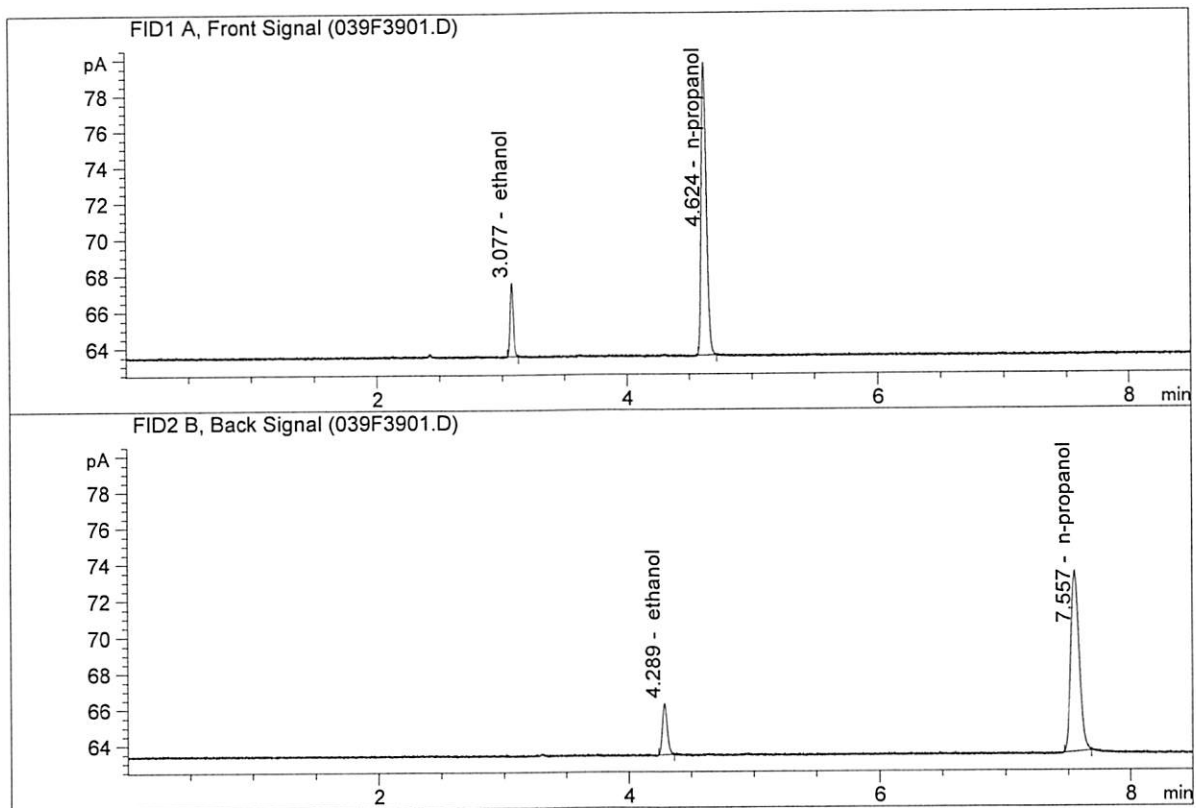


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.44959	0.0814	g/100cc
2.	Ethanol	Column 2:	7.66475	0.0829	g/100cc
3.	n-Propanol	Column 1:	46.11854	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.18966	1.0000	g/100cc

JG

ISP Forensic Services Blood Alcohol Report


Sample Name : QC1-2-B
 Laboratory : Meridian
 Injection Date : Mar 1, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

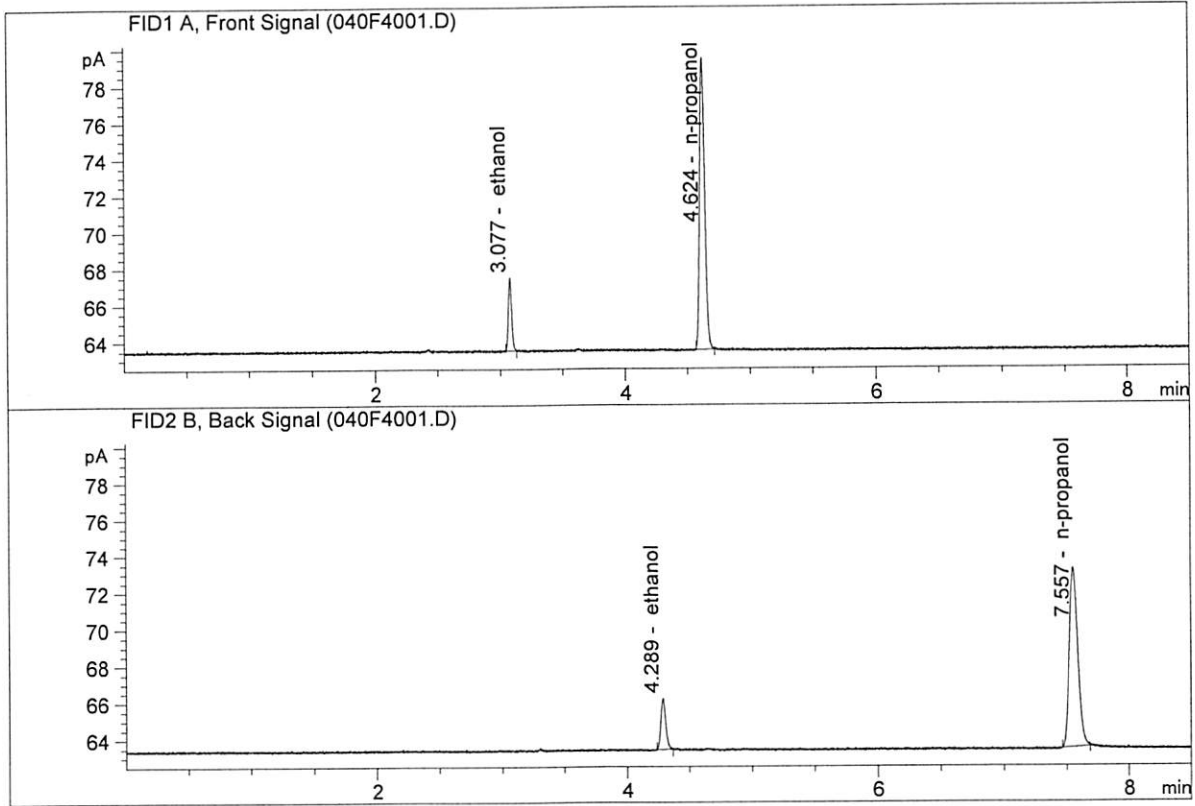

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.25776	0.0807	g/100cc
2.	Ethanol	Column 2:	7.42619	0.0817	g/100cc
3.	n-Propanol	Column 1:	45.29522	1.0000	g/100cc
4.	n-Propanol	Column 2:	46.41978	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STD BLK
 Laboratory : Meridian
 Injection Date : Mar 1, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

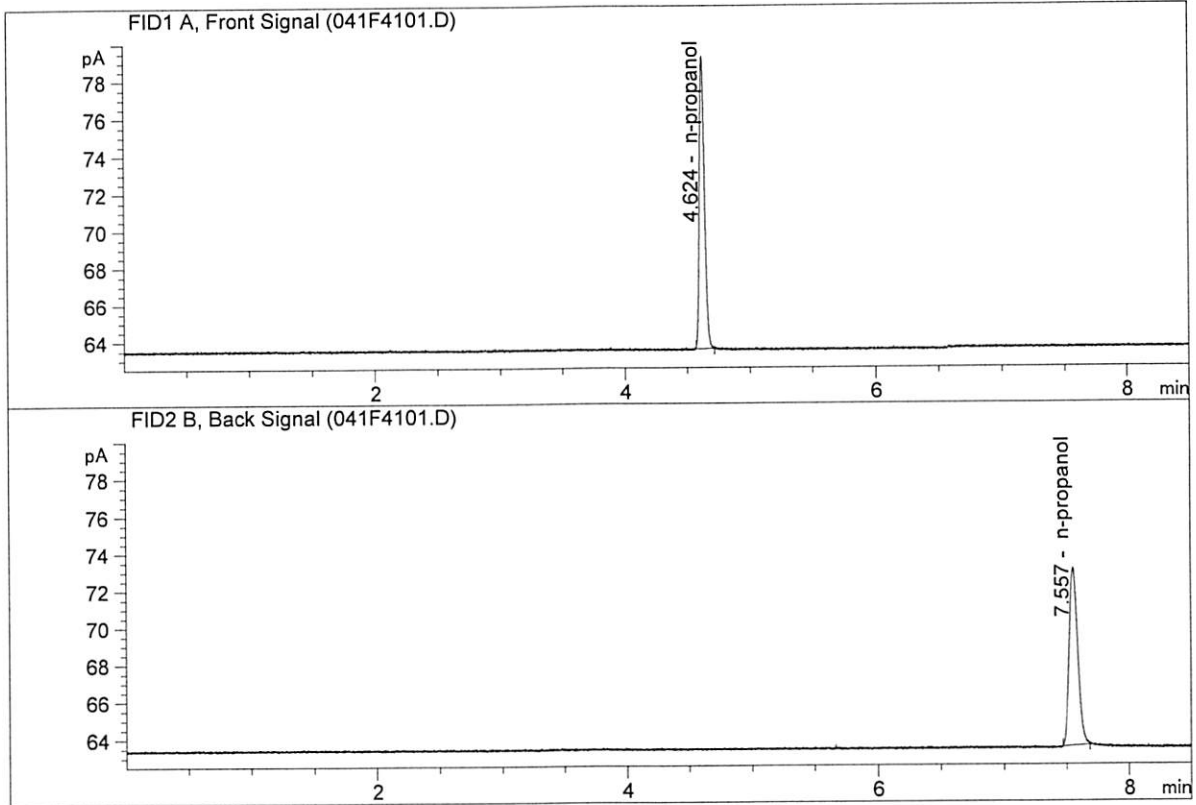

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	44.58944	1.0000	g/100cc
4.	n-Propanol	Column 2:	45.83139	1.0000	g/100cc

S a m p l e S u m m a r y

Sequence table: C:\Chem32\1\Data\03-01-19_SAMPLES\03-01-19_SAMPLES 2019-03-01 14-54-24\03-01-19_SAMPLES.S
 Data directory path: C:\Chem32\1\Data\03-01-19_SAMPLES\03-01-19_SAMPLES 2019-03-01 14-54-24\
 Logbook: C:\Chem32\1\Data\03-01-19_SAMPLES\03-01-19_SAMPLES 2019-03-01 14-54-24\03-01-19_SAMPLES.LOG
 Sequence start: 3/1/2019 3:09:05 PM
 Sequence Operator: SYSTEM
 Operator: SYSTEM

 Method file name: C:\Chem32\1\Data\03-01-19_SAMPLES\03-01-19_SAMPLES 2019-03-01 14-54-24\ALCOHOL.M

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #	Cmp
1	1	1	INTERNAL STD BLK	-	1.0000	001F0101.D		2
2	2	1	MIX VOL FN060415	-	1.0000	002F0201.D		10
3	3	1	QC1-1-A	-	1.0000	003F0301.D		4
4	4	1	QC1-1-B	-	1.0000	004F0401.D		4
5	5	1	0.08 FN04171701-	-	1.0000	005F0501.D		4
6	6	1	0.08 FN04171701-	-	1.0000	006F0601.D		4
7	7	1	M2019-0877-1-A	-	1.0000	007F0701.D		4
8	8	1	M2019-0877-1-B	-	1.0000	008F0801.D		4
9	9	1	M2019-0878-2-A	-	1.0000	009F0901.D		4
10	10	1	M2019-0878-2-B	-	1.0000	010F1001.D		4
11	11	1	M2019-0890-3-A	-	1.0000	011F1101.D		4
12	12	1	M2019-0890-3-B	-	1.0000	012F1201.D		4
13	13	1	M2019-0906-1-A	-	1.0000	013F1301.D		4
14	14	1	M2019-0906-1-B	-	1.0000	014F1401.D		4
15	15	1	M2019-0910-1-A	-	1.0000	015F1501.D		4
16	16	1	M2019-0910-1-B	-	1.0000	016F1601.D		4
17	17	1	M2019-0938-1-A	-	1.0000	017F1701.D		4
18	18	1	M2019-0938-1-B	-	1.0000	018F1801.D		4
19	19	1	M2019-0962-1-A	-	1.0000	019F1901.D		2
20	20	1	M2019-0962-1-B	-	1.0000	020F2001.D		2
21	21	1	M2019-0978-1-A	-	1.0000	021F2101.D		4
22	22	1	M2019-0978-1-B	-	1.0000	022F2201.D		4
23	23	1	M2019-0979-1-A	-	1.0000	023F2301.D		4
24	24	1	M2019-0979-1-B	-	1.0000	024F2401.D		4
25	25	1	QC2-1-A	-	1.0000	025F2501.D		4
26	26	1	QC2-1-B	-	1.0000	026F2601.D		4
27	27	1	M2019-0980-1-A	-	1.0000	027F2701.D		4
28	28	1	M2019-0980-1-B	-	1.0000	028F2801.D		4
29	29	1	M2019-1017-1-A	-	1.0000	029F2901.D		4
30	30	1	M2019-1017-1-B	-	1.0000	030F3001.D		4
31	31	1	M2019-1031-1-A	-	1.0000	031F3101.D		2
32	32	1	M2019-1031-1-B	-	1.0000	032F3201.D		2
33	33	1	M2019-1042-1-A	-	1.0000	033F3301.D		2
34	34	1	M2019-1042-1-B	-	1.0000	034F3401.D		2
35	35	1	M2019-1043-1-A	-	1.0000	035F3501.D		2
36	36	1	M2019-1043-1-B	-	1.0000	036F3601.D		2
37	37	1	M2019-1064-1-A	-	1.0000	037F3701.D		2
38	38	1	M2019-1064-1-B	-	1.0000	038F3801.D		2
39	39	1	QC1-2-A	-	1.0000	039F3901.D		4
40	40	1	QC1-2-B	-	1.0000	040F4001.D		4
41	41	1	INTERNAL STD BLK	-	1.0000	041F4101.D		2

JK

Method file name: C:\Chem32\1\Data\03-01-19_SAMPLES\03-01-19_SAMPLES 2019-03-01 14-54-24
\SHUTDOWN.M

Run #	Location	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #	Cmp
42	42	1	EMPTY	-	1.0000	042F4201.D		0

JC

=====
Calibration Table
=====

General Calibration Setting

Calib. Data Modified : Wednesday, February 20, 2019 2:49:50 PM
Signals calculated separately : No

Rel. Reference Window : 0.000 %
Abs. Reference Window : 0.100 min
Rel. Non-ref. Window : 0.000 %
Abs. Non-ref. Window : 0.100 min
Uncalibrated Peaks : not reported
Partial Calibration : Yes, identified peaks are recalibrated
Correct All Ret. Times: No, only for identified peaks

Curve Type : Linear
Origin : Ignored
Weight : Equal

Recalibration Settings:
Average Response : Average all calibrations
Average Retention Time: Floating Average New 75%

Calibration Report Options :
Printout of recalibrations within a sequence:
 Calibration Table after Recalibration
 Normal Report after Recalibration
If the sequence is done with bracketing:
 Results of first cycle (ending previous bracket)

Default Sample ISTD Information (if not set in sample table):

ISTD #	ISTD Amount [g/100cc]	Name
1	1.00000	n-propanol
2	1.00000	n-propanol

Signal Details

Signal 1: FID1 A, Front Signal
Signal 2: FID2 B, Back Signal

Overview Table

UG

RT	Sig	Lvl	Amount [g/100cc]	Area	Rsp.Factor	Ref	ISTD #	Compound
2.586	1	1	1.00000	3.69669	2.70512e-1	No	No 1	methanol
2.809	1	1	1.00000	4.26100	2.34687e-1	No	No 2	Acetaldehyde
2.977	2	1	1.00000	4.26100	2.34687e-1	No	No 2	Acetaldehyde
3.075	1	1	5.00000e-2	4.50994	1.10866e-2	No	No 1	ethanol
		2	1.00000e-1	9.20050	1.08690e-2			
		3	2.00000e-1	18.63809	1.07307e-2			
		4	3.00000e-1	27.97259	1.07248e-2			
		5	5.00000e-1	47.13963	1.06068e-2			
3.388	2	1	1.00000	4.26062	2.34707e-1	No	No 2	methanol
3.628	1	1	1.00000	9.73055	1.02769e-1	No	No 1	isopropyl alcohol
4.285	2	1	5.00000e-2	4.66614	1.07155e-2	No	No 2	ethanol
		2	1.00000e-1	9.58445	1.04336e-2			
		3	2.00000e-1	19.35337	1.03341e-2			
		4	3.00000e-1	29.33559	1.02265e-2			
		5	5.00000e-1	50.08694	9.98264e-3			
4.308	1	1	1.00000	6.49940	1.53860e-1	No	No 1	acetone
4.620	1	1	1.00000	45.37858	2.20368e-2	No	Yes 1	n-propanol
		2	1.00000	46.75404	2.13885e-2			
		3	1.00000	46.87068	2.13353e-2			
		4	1.00000	46.59780	2.14602e-2			
		5	1.00000	47.42130	2.10876e-2			
4.661	2	1	1.00000	6.89301	1.45075e-1	No	No 2	acetone
4.969	2	1	1.00000	10.70642	9.34019e-2	No	No 2	isopropyl alcohol
7.550	2	1	1.00000	47.42397	2.10864e-2	No	Yes 2	n-propanol
		2	1.00000	48.55627	2.05947e-2			
		3	1.00000	48.39064	2.06652e-2			
		4	1.00000	48.12415	2.07796e-2			
		5	1.00000	48.76479	2.05066e-2			


Peak Sum Table

No Entries in table

1 Warnings or Errors :


Warning : Curve requires more calibration points., (methanol)

Calibration Curves

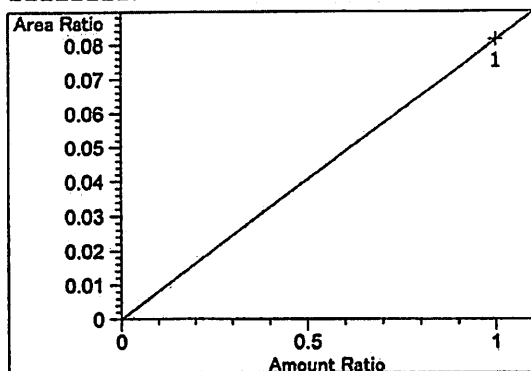


methanol at exp. RT: 2.586
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 8.14634e-2
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio


36

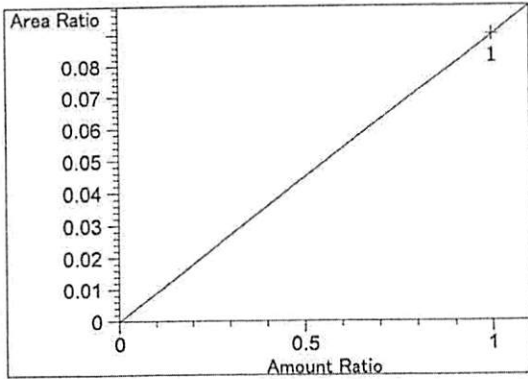


Acetaldehyde at exp. RT: 2.809
FID1 A, Front Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx + b$
m: 8.98491e-2
b: 0.00000
x: Amount Ratio
y: Area Ratio

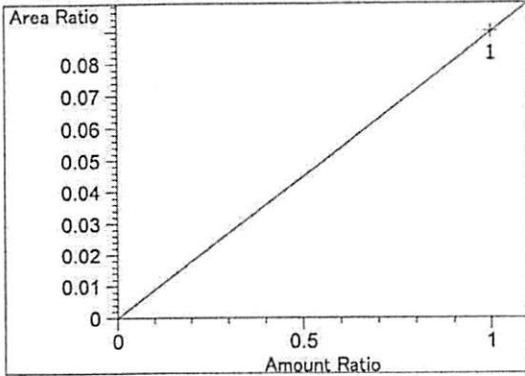

Acetaldehyde at exp. RT: 2.977
FID2 B, Back Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx + b$
m: 8.98491e-2
b: 0.00000
x: Amount Ratio
y: Area Ratio

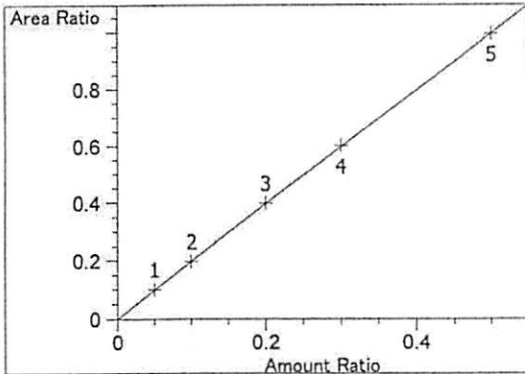


ethanol at exp. RT: 3.075
FID1 A, Front Signal
Correlation: 0.99998
Residual Std. Dev.: 0.00232
Formula: $y = mx + b$
m: 1.99232
b: -5.96924e-4
x: Amount Ratio
y: Area Ratio

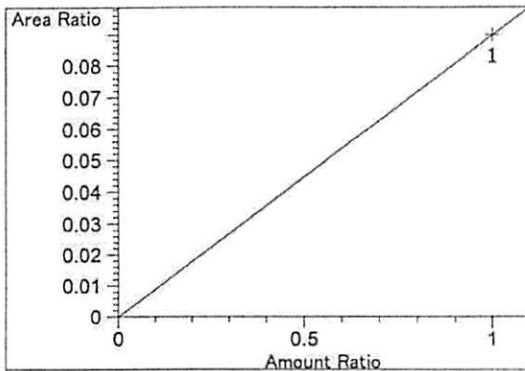


methanol at exp. RT: 3.388
FID2 B, Back Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx + b$
m: 8.98412e-2
b: 0.00000
x: Amount Ratio
y: Area Ratio


J6

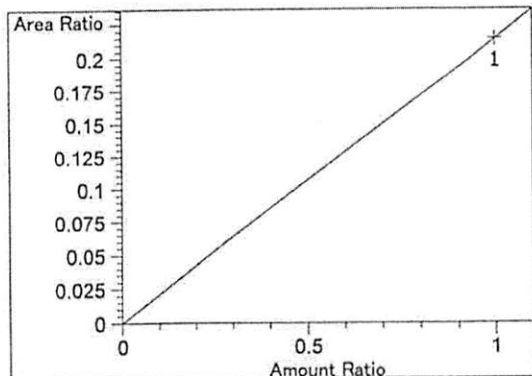


isopropyl alcohol at exp. RT: 3.628
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 2.14431e-1
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio

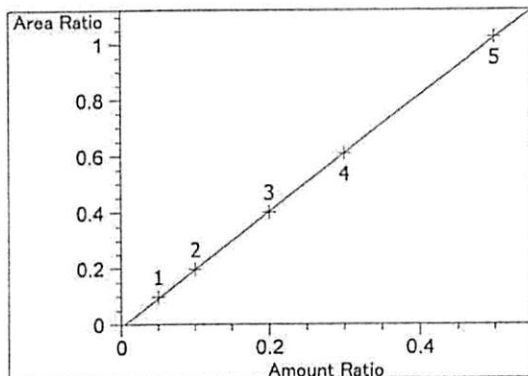

ethanol at exp. RT: 4.285
 FID2 B, Back Signal
 Correlation: 0.99996
 Residual Std. Dev.: 0.00389
 Formula: $y = mx + b$
 m: 2.06736
 b: -9.00937e-3
 x: Amount Ratio
 y: Area Ratio

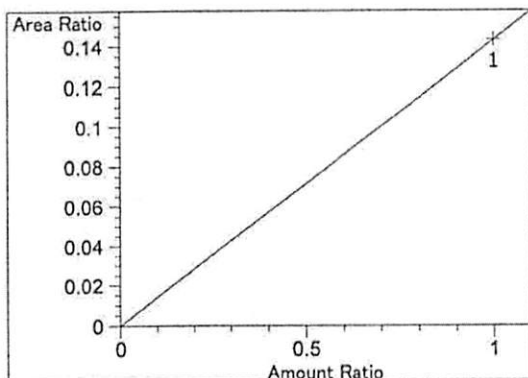


acetone at exp. RT: 4.308
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 1.43226e-1
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio

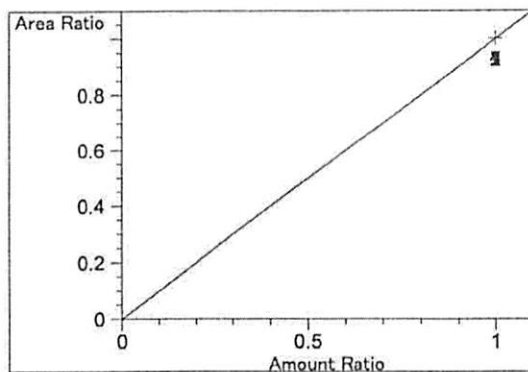


n-propanol at exp. RT: 4.620
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 1.00000
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio


dg

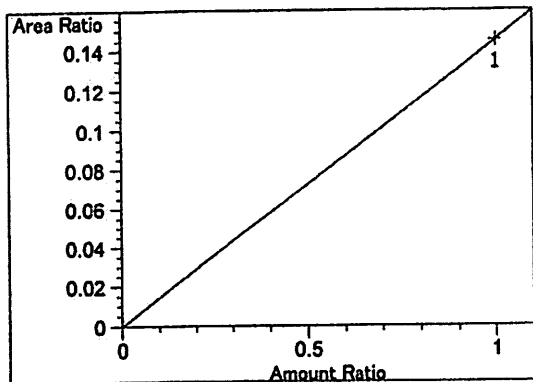

acetone at exp. RT: 4.661
FID2 B, Back Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx + b$
m: 1.45349e-1
b: 0.00000
x: Amount Ratio
y: Area Ratio

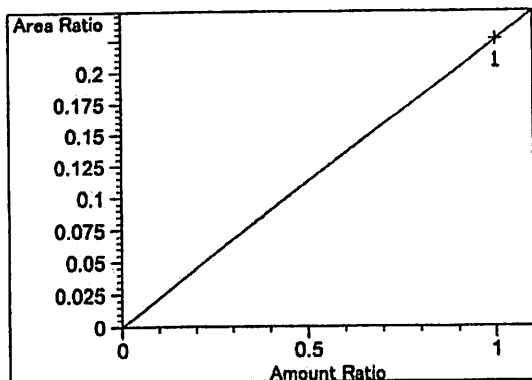

isopropyl alcohol at exp. RT: 4.969
FID2 B, Back Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx + b$
m: 2.25760e-1
b: 0.00000
x: Amount Ratio
y: Area Ratio

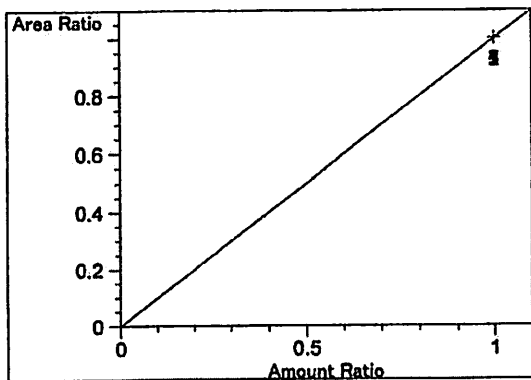


n-propanol at exp. RT: 7.550
FID2 B, Back Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx + b$
m: 1.00000
b: 0.00000
x: Amount Ratio
y: Area Ratio

=====

JG

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.050 FN04271601
 Laboratory : Meridian
 Injection Date : Feb 20, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

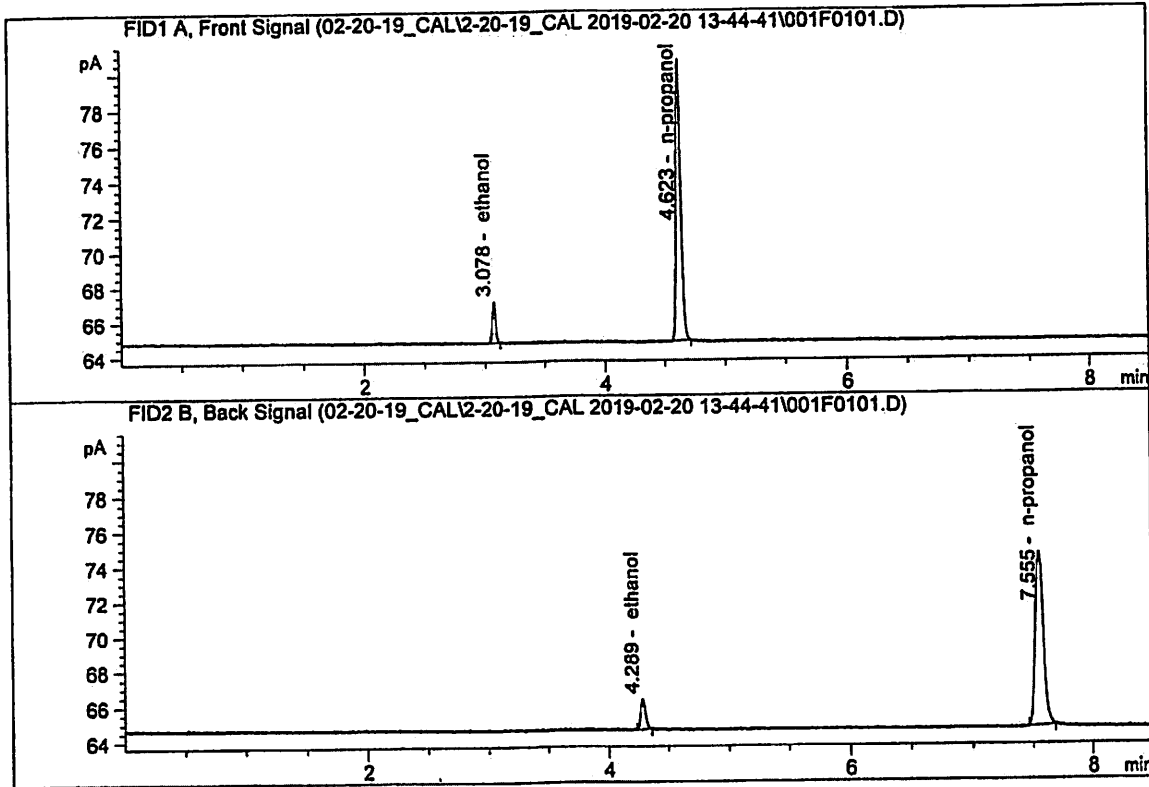


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	4.50994	0.0502	g/100cc
2.	Ethanol	Column 2:	4.66614	0.0520	g/100cc
3.	n-Propanol	Column 1:	45.37858	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.42397	1.0000	g/100cc

JK

ISP Forensic Services Blood Alcohol Report


Sample Name : 0.100 FN08101601
 Laboratory : Meridian
 Injection Date : Feb 20, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

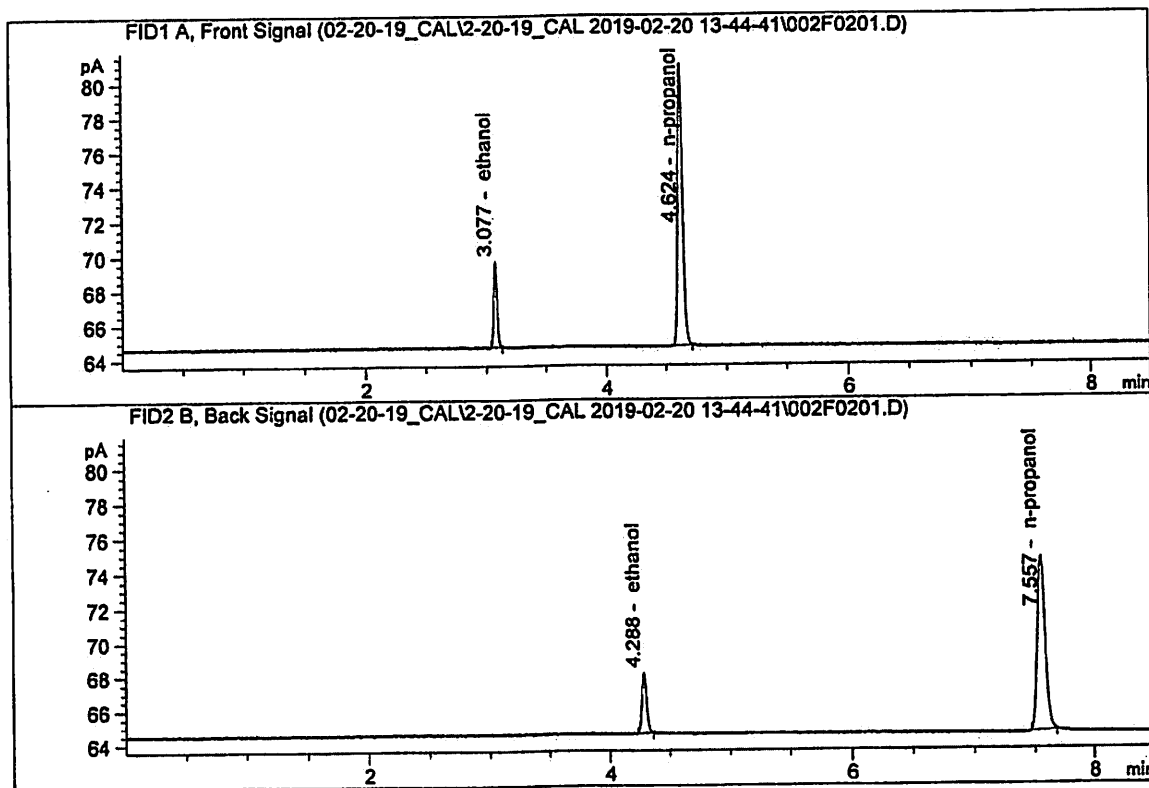

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	9.20050	0.0991	g/100cc
2.	Ethanol	Column 2:	9.58445	0.0998	g/100cc
3.	n-Propanol	Column 1:	46.75404	1.0000	g/100cc
4.	n-Propanol	Column 2:	48.55627	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.200 FN03301601
 Laboratory : Meridian
 Injection Date : Feb 20, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

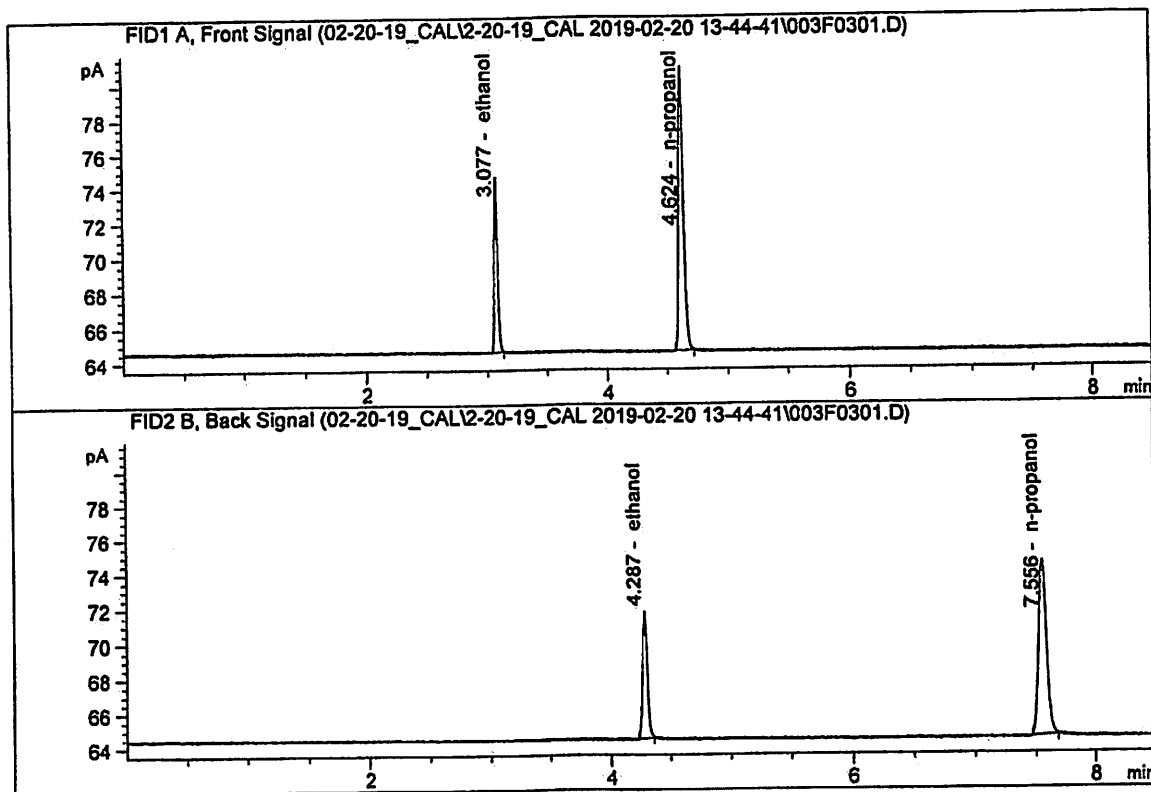


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	18.63809	0.1999	g/100cc
2.	Ethanol	Column 2:	19.35337	0.1978	g/100cc
3.	n-Propanol	Column 1:	46.87068	1.0000	g/100cc
4.	n-Propanol	Column 2:	48.39064	1.0000	g/100cc

JG

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.300 FN02121601
 Laboratory : Meridian
 Injection Date : Feb 20, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

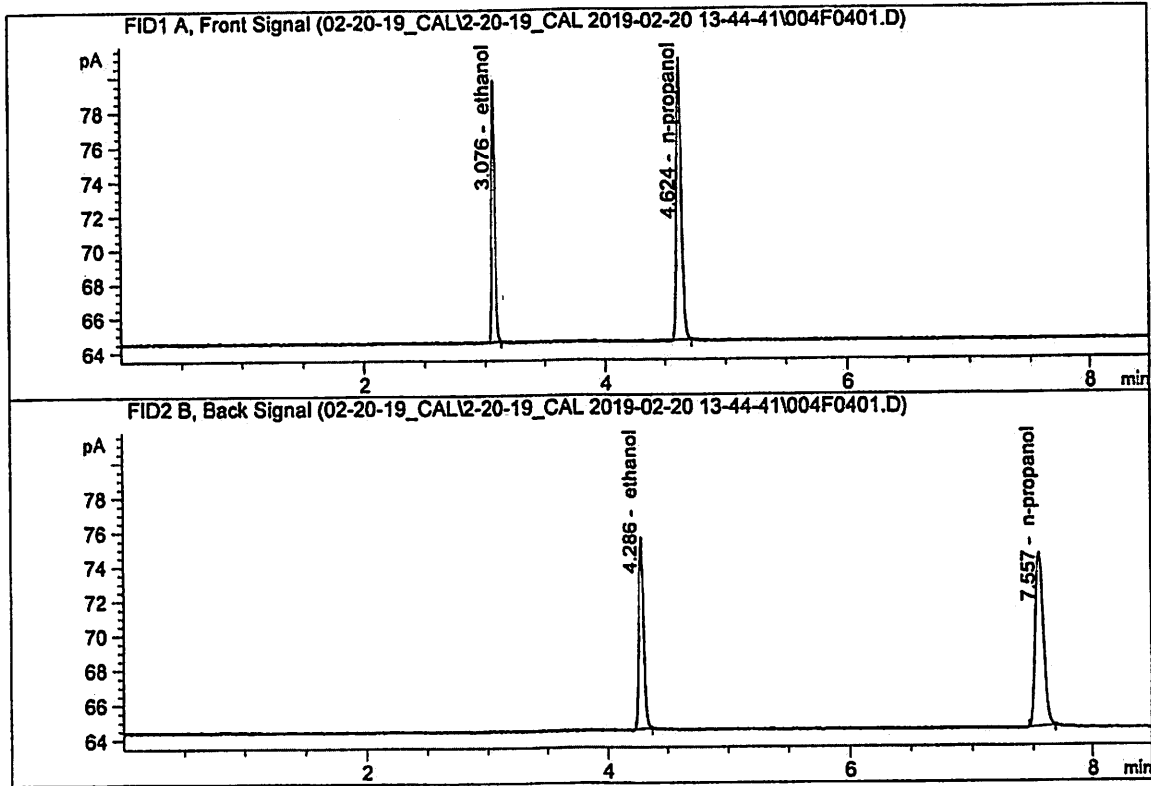


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	27.97259	0.3016	g/100cc
2.	Ethanol	Column 2:	29.33559	0.2992	g/100cc
3.	n-Propanol	Column 1:	46.59780	1.0000	g/100cc
4.	n-Propanol	Column 2:	48.12415	1.0000	g/100cc

JG

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.500 FN08031602
 Laboratory : Meridian
 Injection Date : Feb 20, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

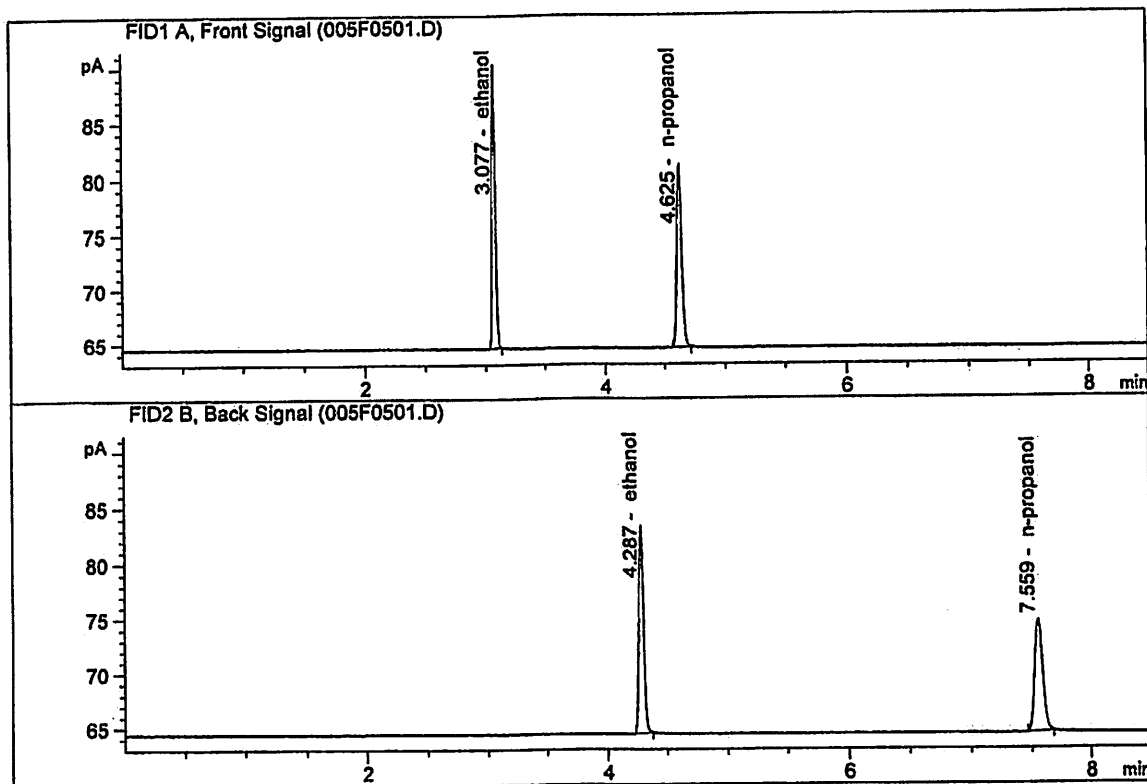


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	47.13963	0.4992	g/100cc
2.	Ethanol	Column 2:	50.08694	0.5012	g/100cc
3.	n-Propanol	Column 1:	47.42130	1.0000	g/100cc
4.	n-Propanol	Column 2:	48.76479	1.0000	g/100cc

JG

ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STANDARD BLANK
 Laboratory : Meridian
 Injection Date : Feb 20, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

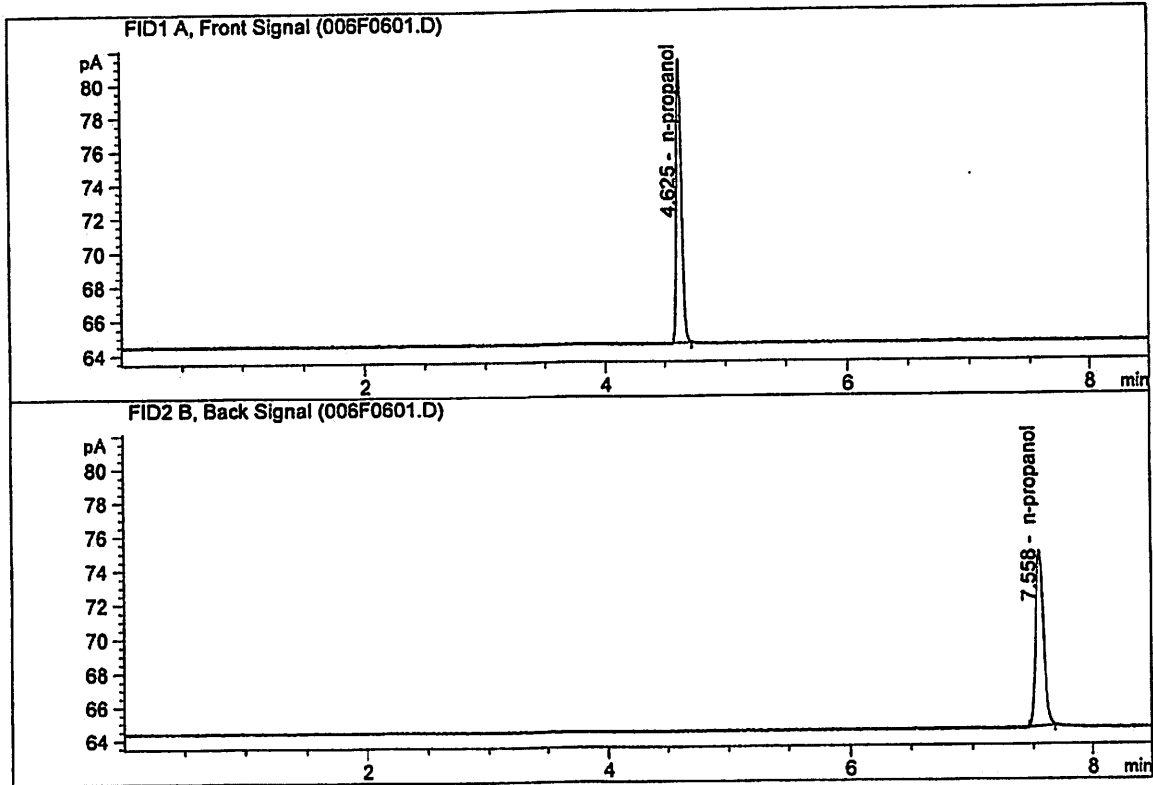

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	47.92826	1.0000	g/100cc
4.	n-Propanol	Column 2:	49.58934	1.0000	g/100cc

dg

S a m p l e S u m m a r y

Sequence table: C:\Chem32\1\Data\02-20-19_CAL\2-20-19_CAL 2019-02-20 13-44-41\2-20-19_CAL
S
 Data directory path: C:\Chem32\1\Data\02-20-19_CAL\2-20-19_CAL 2019-02-20 13-44-41\
 Logbook: C:\Chem32\1\Data\02-20-19_CAL\2-20-19_CAL 2019-02-20 13-44-41\2-20-19_CAL
 LOG
 Sequence start: 2/20/2019 1:59:18 PM
 Sequence Operator: SYSTEM
 Operator: SYSTEM
 Method file name: C:\Chem32\1\Data\02-20-19_CAL\2-20-19_CAL 2019-02-20 13-44-41\ALCOHOL.M

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #	# Cmp
1	1	1	0.050 FN04271601	-	1.0000	001F0101.D	*	4
2	2	1	0.100 FN08101601	-	1.0000	002F0201.D	*	4
3	3	1	0.200 FN03301601	-	1.0000	003F0301.D	*	4
4	4	1	0.300 FN02121601	-	1.0000	004F0401.D	*	4
5	5	1	0.500 FN08031602	-	1.0000	005F0501.D	*	4
6	6	1	INTERNAL STANDAR	-	1.0000	006F0601.D		2

26