
















REVIEWED

By Anne Nord at 11:20 am, Mar 08, 2019

3/8/2019

Worklist: 3019

<u>LAB CASE</u>	<u>ITEM</u>	<u>TASK ID</u>	<u>DESCRIPTION</u>	
M2019-0876	4	143032	Alcohol Analysis	
P2019-0625	1	142875	Alcohol Analysis	
P2019-0627	1	142879	Alcohol Analysis	
P2019-0632	1	142887	Alcohol Analysis	
P2019-0645	1	143025	Alcohol Analysis	
P2019-0657	1	143188	Alcohol Analysis	
P2019-0664	1	143199	Alcohol Analysis	
P2019-0665	1	143200	Alcohol Analysis	
P2019-0668	2	143210	Alcohol Analysis	
P2019-0671	1	143236	Alcohol Analysis	
P2019-0672	1	143237	Alcohol Analysis	
P2019-0673	1	143238	Alcohol Analysis	
P2019-0674	1	143239	Alcohol Analysis	
P2019-0685	1	143284	Alcohol Analysis	
P2019-0686	1	143288	Alcohol Analysis	
P2019-0707	1	143623	Alcohol Analysis	
P2019-0708	1	143664	Alcohol Analysis	
P2019-0709	1	143665	Alcohol Analysis	
P2019-0736	1	143803	Alcohol Analysis	
P2019-0737	1	143807	Alcohol Analysis	
P2019-0737	2	143811	Alcohol Analysis	



Worklist: 3021

<u>LAB CASE</u>	<u>ITEM</u>	<u>TASK ID</u>	<u>DESCRIPTION</u>
M2019-0626	1	143926	Alcohol Analysis



*AC*₁

Quantitative Analysis for Ethanol & Qualitative Analysis for Other Volatiles

Analytical Method(s): 1.0

Device: Hamilton MICROLAB 503A Liquid Processor/Dilutor Serial Number: MD96BC1382

Volatiles Quality Assurance Controls

Run Date(s): 3/7/19

Curve on 2/27/19

Control Level	Expiration	Lot #	Target Value	Acceptable Range	Overall Results
Level 1	Jan-22	1801036	0.0812	0.0731 - 0.0893	0.0762 g/100cc
					0.0781 g/100cc
					g/100cc
Level 2	Mar-22	1803028	0.2035	0.1832 - 0.2238	0.1960 g/100cc 0.2012 g/100cc g/100cc
Multi-Component mixture:					
Curve Fit:		Column 1	Lot #	Column 2	
			0.99997		11918 0.99996

Ethanol Calibration Reference Material						
Calibrator level	Target Value	Acceptable Range	Column 1	Column 2	Precision	Mean
50	0.050	0.045 - 0.055	0.0479	0.0489	0.001	0.0484
100	0.100	0.090 - 0.110	0.0972	0.0970	0.0002	0.0971
200	0.200	0.180 - 0.220	0.1980	0.1974	0.0006	0.1977
300	0.300	0.270 - 0.330	0.2982	0.2975	0.0007	0.2978
500	0.500	0.450 - 0.550	0.5027	0.5032	0.0005	0.5029

Aqueous Controls			
Control level	Target Value	Acceptable Range	Overall Results
80	0.080	0.076 - 0.084	0.077 g/100cc

Revision: 1

Issue Date: 01/03/2019

=====
Calibration Table
=====-----
General Calibration Setting

Calib. Data Modified : Wednesday, February 27, 2019 1:30:44 PM

Signals calculated separately : No

Rel. Reference Window : 0.000 %
Abs. Reference Window : 0.100 min
Rel. Non-ref. Window : 0.000 %
Abs. Non-ref. Window : 0.100 min
Uncalibrated Peaks : not reported
Partial Calibration : No recalibration if peaks missing

Curve Type : Linear
Origin : Forced
Weight : Equal

Recalibration Settings:
Average Response : Average all calibrations
Average Retention Time: Floating Average New 75%

Calibration Report Options :

Printout of recalibrations within a sequence:

Calibration Table after Recalibration

Normal Report after Recalibration

If the sequence is done with bracketing:

Results of first cycle (ending previous bracket)

Default Sample ISTD Information (if not set in sample table):

ISTD #	ISTD Amount [g/100cc]	Name
1	1.00000	n-Propanol
2	1.00000	n-Propanol

Signal Details

Signal 1: FID1 A, Front Signal


Signal 2: FID2 B, Back Signal

Overview Table


RT	Sig	Lvl	Amount [g/100cc]	Area	Rsp.Factor	Ref	ISTD #	Compound
2.227	2	1	1.00000	6.45200	1.54991e-1	No	No 2	Fluorinated ethane
2.271	1	1	1.00000	1.84105	5.43168e-1	No	No 1	Fluorinated ethane
2.685	1	1	1.00000	3.69669	2.70512e-1	No	No 1	Methanol
2.950	2	1	1.00000	11.54700	8.66026e-2	No	No 2	Acetaldehyde
2.975	1	1	1.00000	10.52400	9.50209e-2	No	No 1	Acetaldehyde
3.317	1	1	5.00000e-2	11.08207	4.51179e-3	No	No 1	Ethanol
		2	1.00000e-1	22.61685	4.42148e-3			
		3	2.00000e-1	48.20628	4.14884e-3			
		4	3.00000e-1	69.12797	4.33978e-3			
		5	5.00000e-1	117.86619	4.24210e-3			
3.372	2	1	1.00000	4.26062	2.34707e-1	No	No 2	Methanol
3.993	1	1	1.00000	9.73055	1.02769e-1	No	No 1	Isopropyl alcohol
4.334	2	1	5.00000e-2	11.24602	4.44602e-3	No	No 2	Ethanol
		2	1.00000e-1	22.35963	4.47235e-3			
		3	2.00000e-1	47.20350	4.23697e-3			
		4	3.00000e-1	67.68433	4.43234e-3			
		5	5.00000e-1	115.28214	4.33719e-3			
4.704	2	1	1.00000	6.89301	1.45075e-1	No	No 2	Acetone
4.853	1	1	1.00000	6.49940	1.53860e-1	No	No 1	Acetone
5.050	2	1	1.00000	10.70642	9.34019e-2	No	No 2	Isopropyl alcohol
5.259	1	1	1.00000	133.72021	7.47830e-3	No	Yes 1	n-Propanol
		2	1.00000	134.42337	7.43918e-3			
		3	1.00000	140.65019	7.10984e-3			
		4	1.00000	133.94193	7.46592e-3			
		5	1.00000	135.46065	7.38222e-3			
		6	1.00000	111.45872	8.97193e-3			
7.659	2	1	1.00000	5.98700	1.67029e-1	No	No 2	Ethyl Acetate
7.789	2	1	1.00000	135.89790	7.35847e-3	No	Yes 2	n-Propanol
		2	1.00000	136.19337	7.34250e-3			
		3	1.00000	141.33327	7.07548e-3			
		4	1.00000	134.49538	7.43520e-3			
		5	1.00000	135.41518	7.38470e-3			
		6	1.00000	113.50471	8.81021e-3			
8.420	1	1	1.00000	5.56500	1.79695e-1	No	No 1	Ethyl Acetate
11.631	2	1	1.00000	864.84247	1.15628e-3	No	No 2	Toluene
12.229	1	1	1.00000	918.48389	1.08875e-3	No	No 1	Toluene

Peak Sum Table


No Entries in table

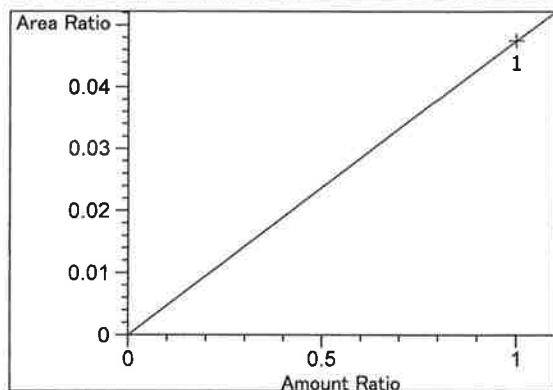=====
=====
Calibration Curves
=====


Fluorinated ethane at exp. RT: 2.227
FID2 B, Back Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx$
m: $4.74768e-2$
x: Amount Ratio
y: Area Ratio

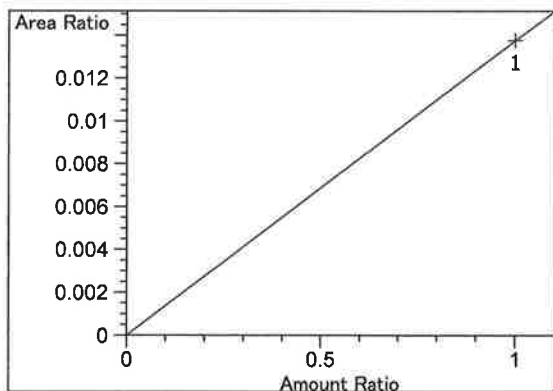


Fluorinated ethane at exp. RT: 2.271
FID1 A, Front Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx$
m: $1.37679e-2$
x: Amount Ratio
y: Area Ratio

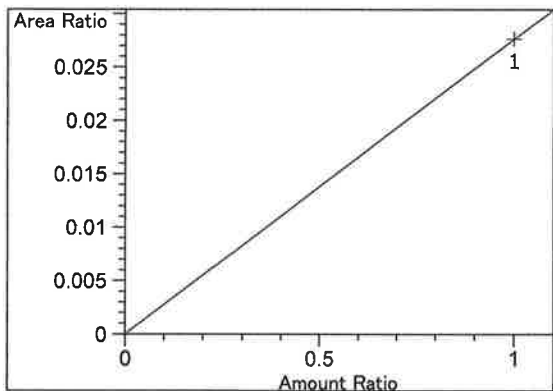


Methanol at exp. RT: 2.685
FID1 A, Front Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx$
m: $2.76450e-2$
x: Amount Ratio
y: Area Ratio

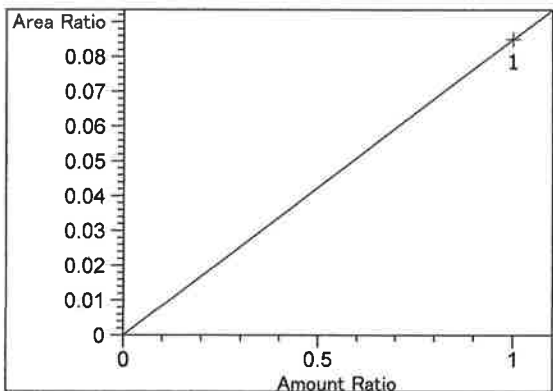


Acetaldehyde at exp. RT: 2.950
FID2 B, Back Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx$
m: $8.49682e-2$
x: Amount Ratio
y: Area Ratio

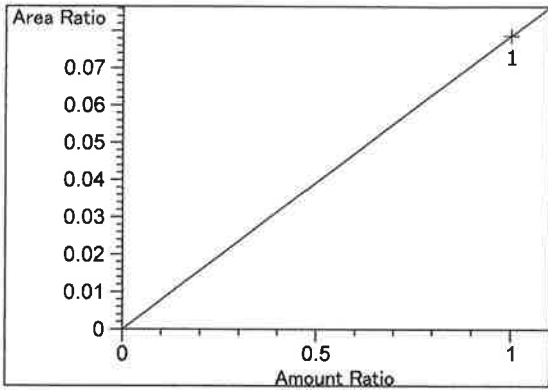


Acetaldehyde at exp. RT: 2.975
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx$
 m: $7.87016e-2$
 x: Amount Ratio
 y: Area Ratio

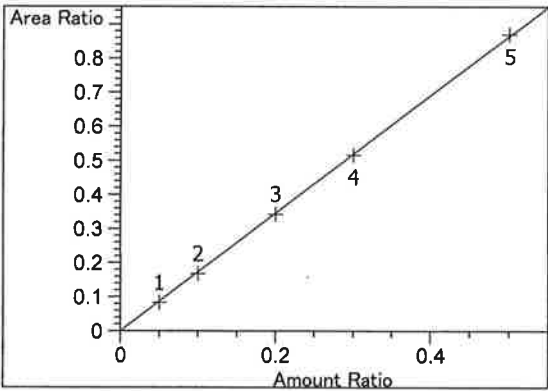

Ethanol at exp. RT: 3.317
 FID1 A, Front Signal
 Correlation: 0.99997
 Residual Std. Dev.: 0.00449
 Formula: $y = mx$
 m: 1.73097
 x: Amount Ratio
 y: Area Ratio

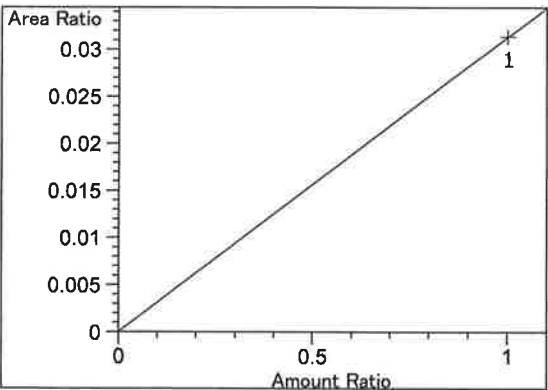


Methanol at exp. RT: 3.372
 FID2 B, Back Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx$
 m: $3.13517e-2$
 x: Amount Ratio
 y: Area Ratio

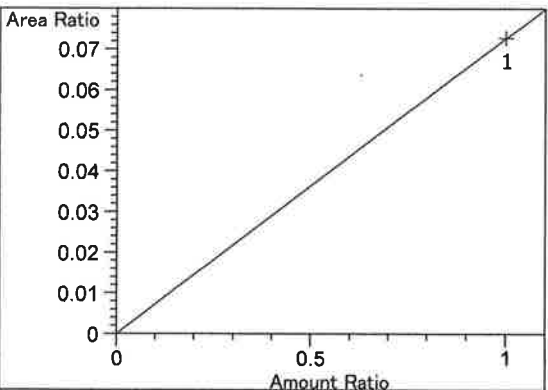


Isopropyl alcohol at exp. RT: 3.993
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx$
 m: $7.27680e-2$
 x: Amount Ratio
 y: Area Ratio


RC

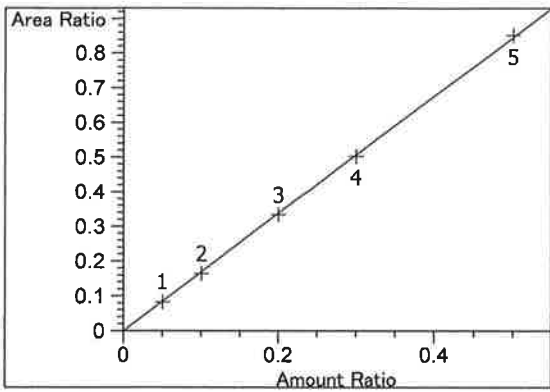


Ethanol at exp. RT: 4.334
 FID2 B, Back Signal
 Correlation: 0.99996
 Residual Std. Dev.: 0.00488
 Formula: $y = mx$
 m: 1.69169
 x: Amount Ratio
 y: Area Ratio

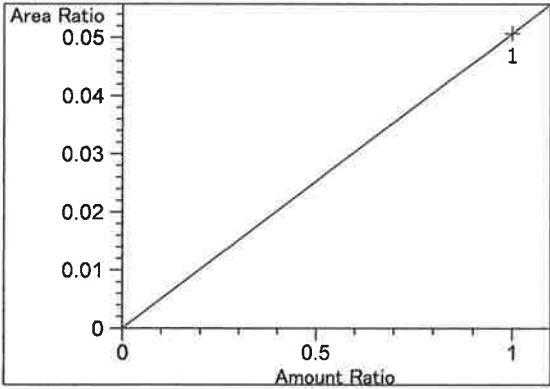

Acetone at exp. RT: 4.704
 FID2 B, Back Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx$
 m: 5.07220e-2
 x: Amount Ratio
 y: Area Ratio

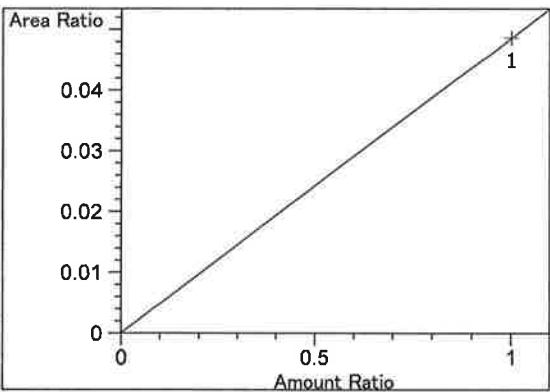


Acetone at exp. RT: 4.853
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx$
 m: 4.86045e-2
 x: Amount Ratio
 y: Area Ratio

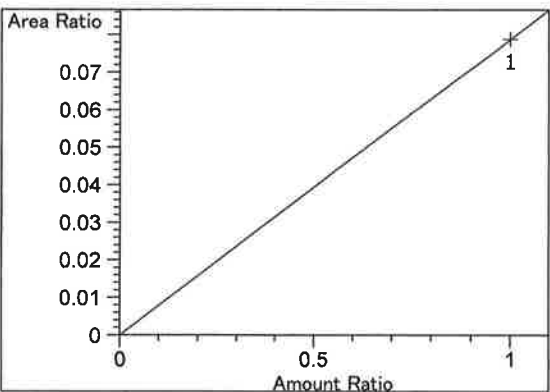


Isopropyl alcohol at exp. RT: 5.050
 FID2 B, Back Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx$
 m: 7.87828e-2
 x: Amount Ratio
 y: Area Ratio


Handwritten signature

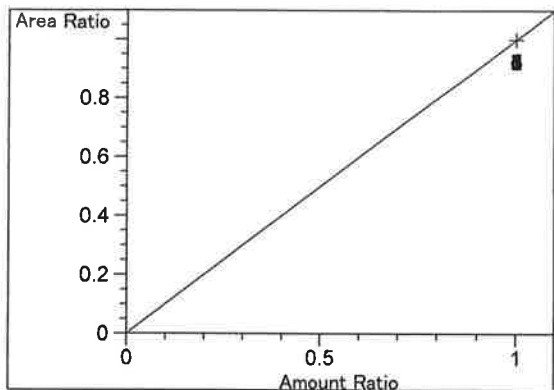


n-Propanol at exp. RT: 5.259
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx$
 m: 1.00000
 x: Amount Ratio
 y: Area Ratio

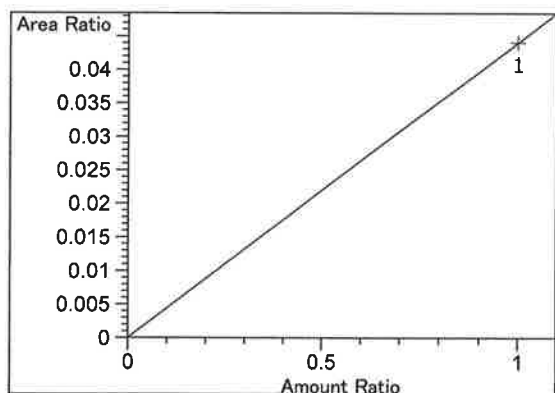

Ethyl Acetate at exp. RT: 7.659
 FID2 B, Back Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx$
 m: 4.40551e-2
 x: Amount Ratio
 y: Area Ratio

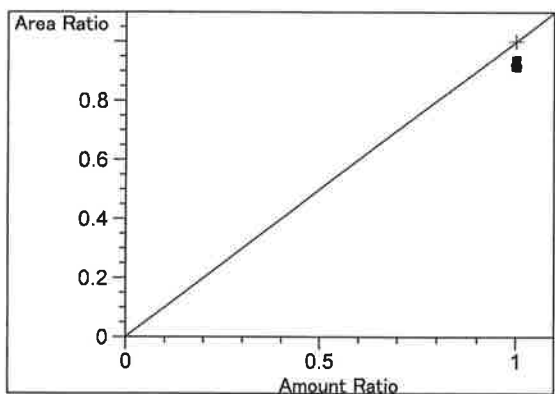


n-Propanol at exp. RT: 7.789
 FID2 B, Back Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx$
 m: 1.00000
 x: Amount Ratio
 y: Area Ratio

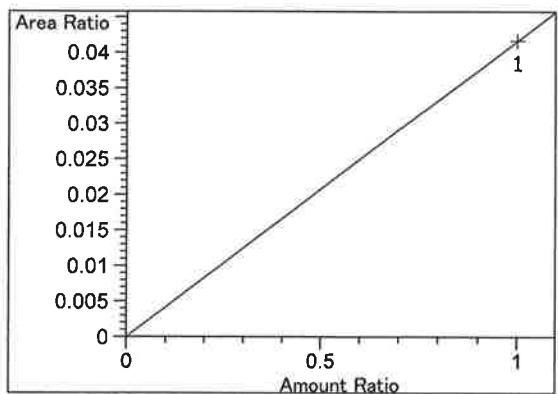


Ethyl Acetate at exp. RT: 8.420
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx$
 m: 4.16167e-2
 x: Amount Ratio
 y: Area Ratio

RC

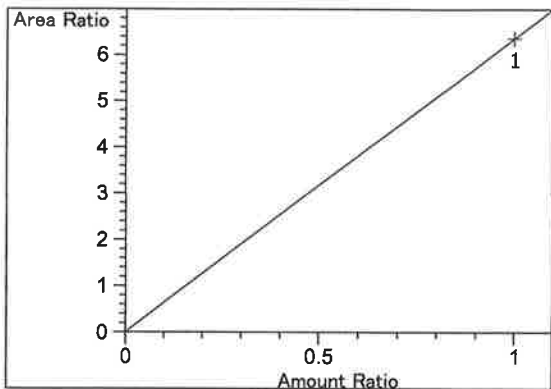

Toluene at exp. RT: 11.631
FID2 B, Back Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx$
m: 6.36391
x: Amount Ratio
y: Area Ratio

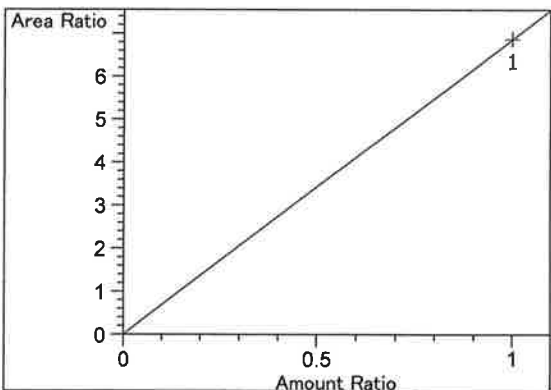


Toluene at exp. RT: 12.229
FID1 A, Front Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx$
m: 6.86870
x: Amount Ratio
y: Area Ratio

RC

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.05
 Laboratory : Pocatello
 Injection Date : Feb 27, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN10742043-IT00741010

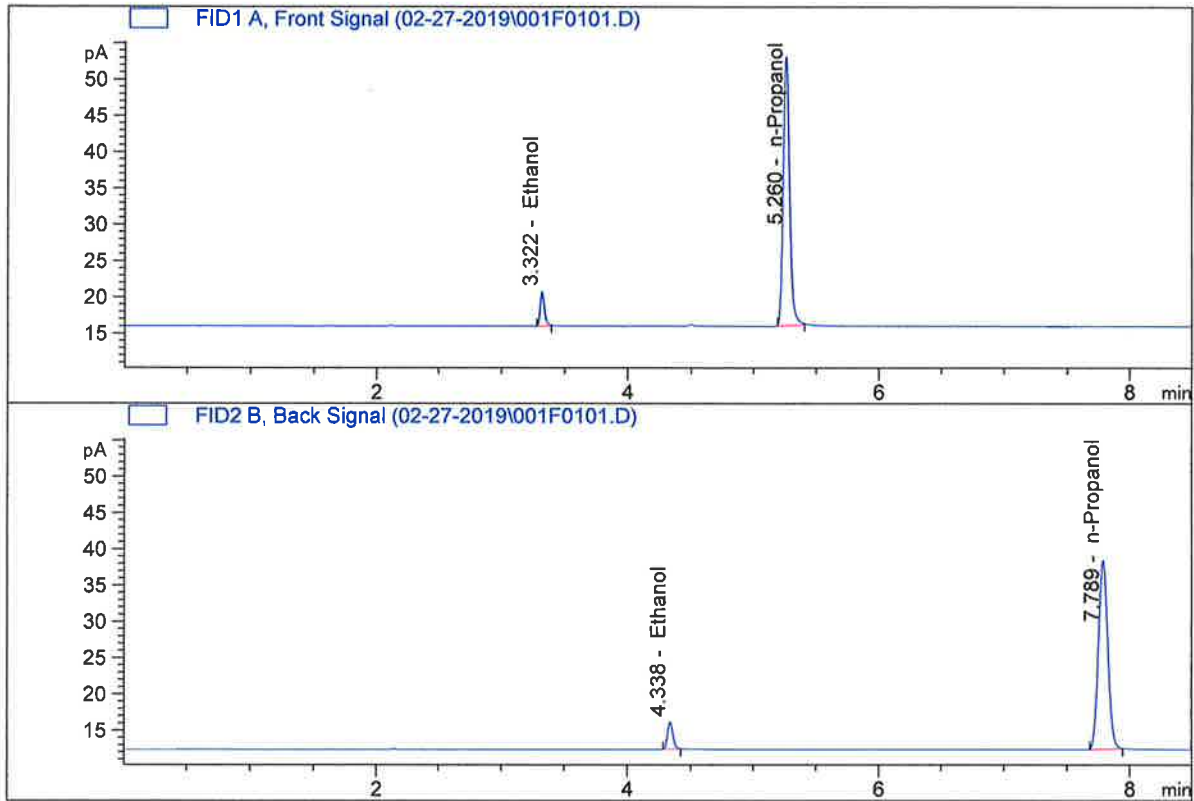


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	11.08207	0.0479	g/100cc
2.	Ethanol	Column 2:	11.24602	0.0489	g/100cc
3.	n-Propanol	Column 1:	133.72021	1.0000	g/100cc
4.	n-Propanol	Column 2:	135.89790	1.0000	g/100cc

YFC

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.10
 Laboratory : Pocatello
 Injection Date : Feb 27, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN10742043-IT00741010

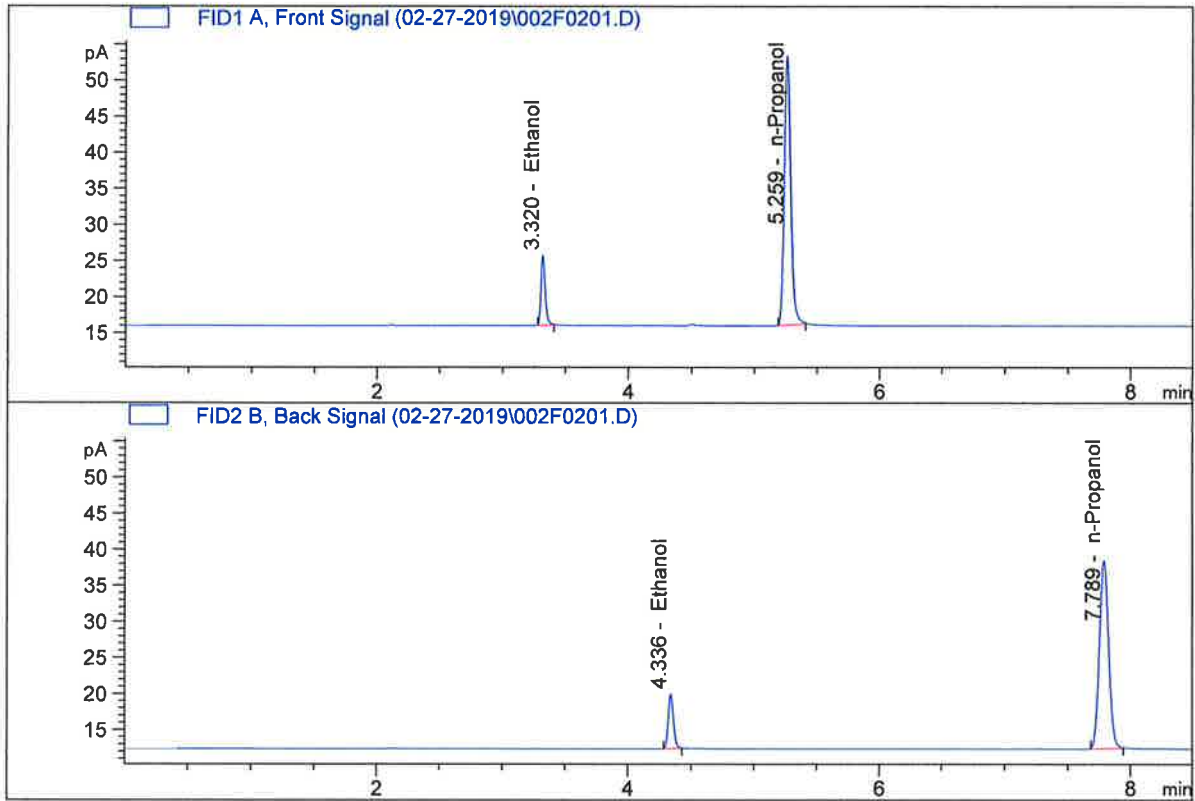


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	22.61685	0.0972	g/100cc
2.	Ethanol	Column 2:	22.35963	0.0970	g/100cc
3.	n-Propanol	Column 1:	134.42337	1.0000	g/100cc
4.	n-Propanol	Column 2:	136.19337	1.0000	g/100cc

RC

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.20
 Laboratory : Pocatello
 Injection Date : Feb 27, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN10742043-IT00741010

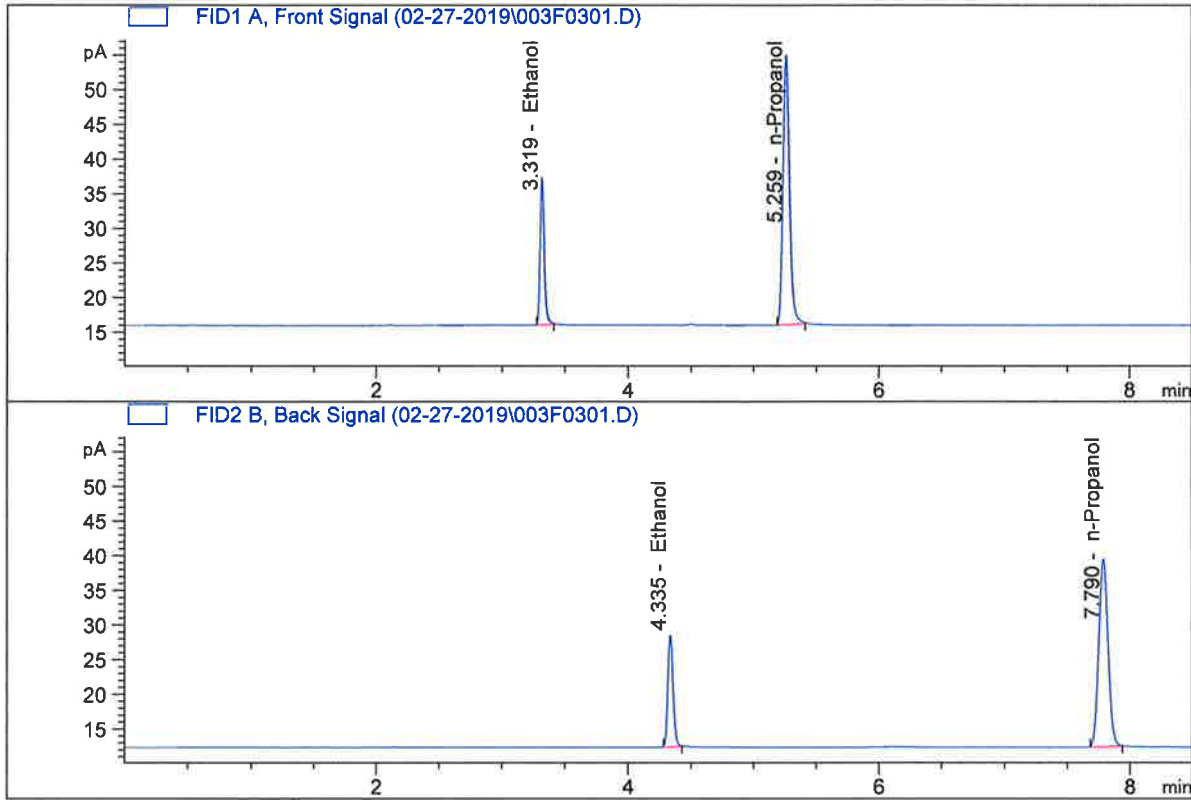


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	48.20628	0.1980	g/100cc
2.	Ethanol	Column 2:	47.20350	0.1974	g/100cc
3.	n-Propanol	Column 1:	140.65019	1.0000	g/100cc
4.	n-Propanol	Column 2:	141.33327	1.0000	g/100cc

PC

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.300
 Laboratory : Pocatello
 Injection Date : Feb 27, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN10742043-IT00741010

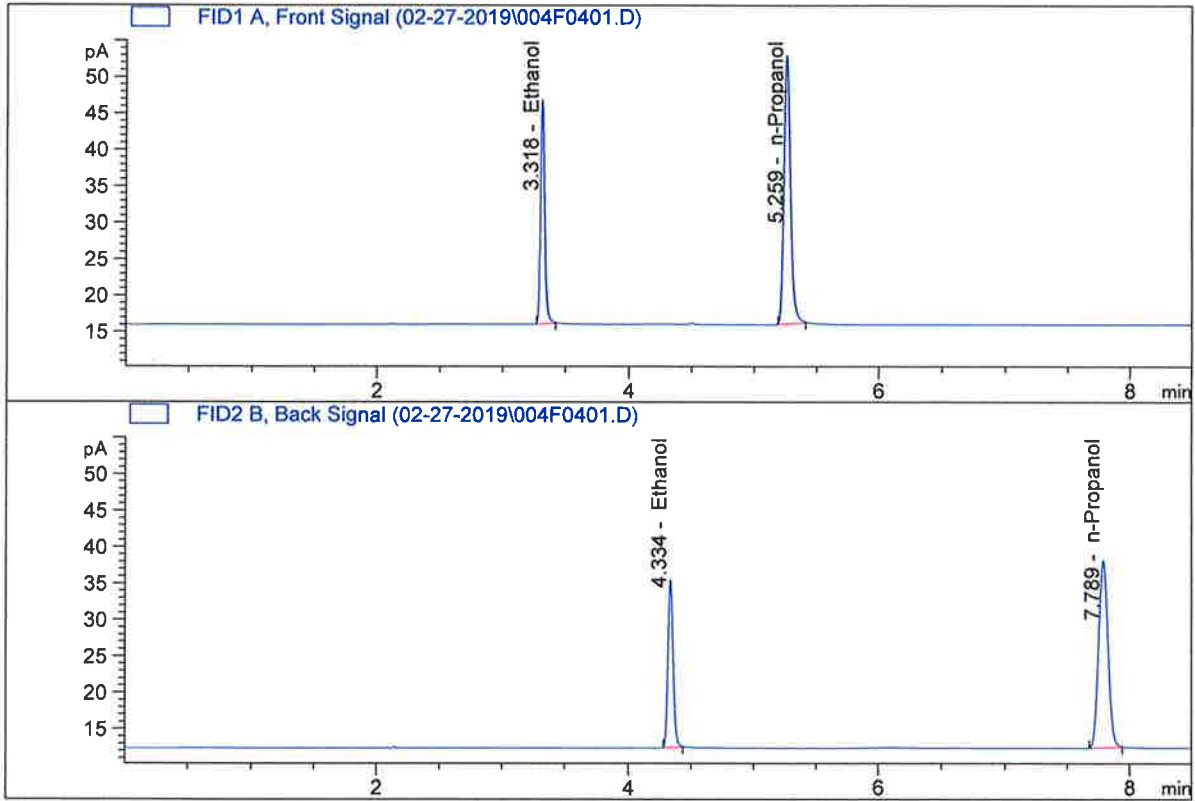


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	69.12797	0.2982	g/100cc
2.	Ethanol	Column 2:	67.68433	0.2975	g/100cc
3.	n-Propanol	Column 1:	133.94193	1.0000	g/100cc
4.	n-Propanol	Column 2:	134.49538	1.0000	g/100cc

AC

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.50
 Laboratory : Pocatello
 Injection Date : Feb 27, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN10742043-IT00741010

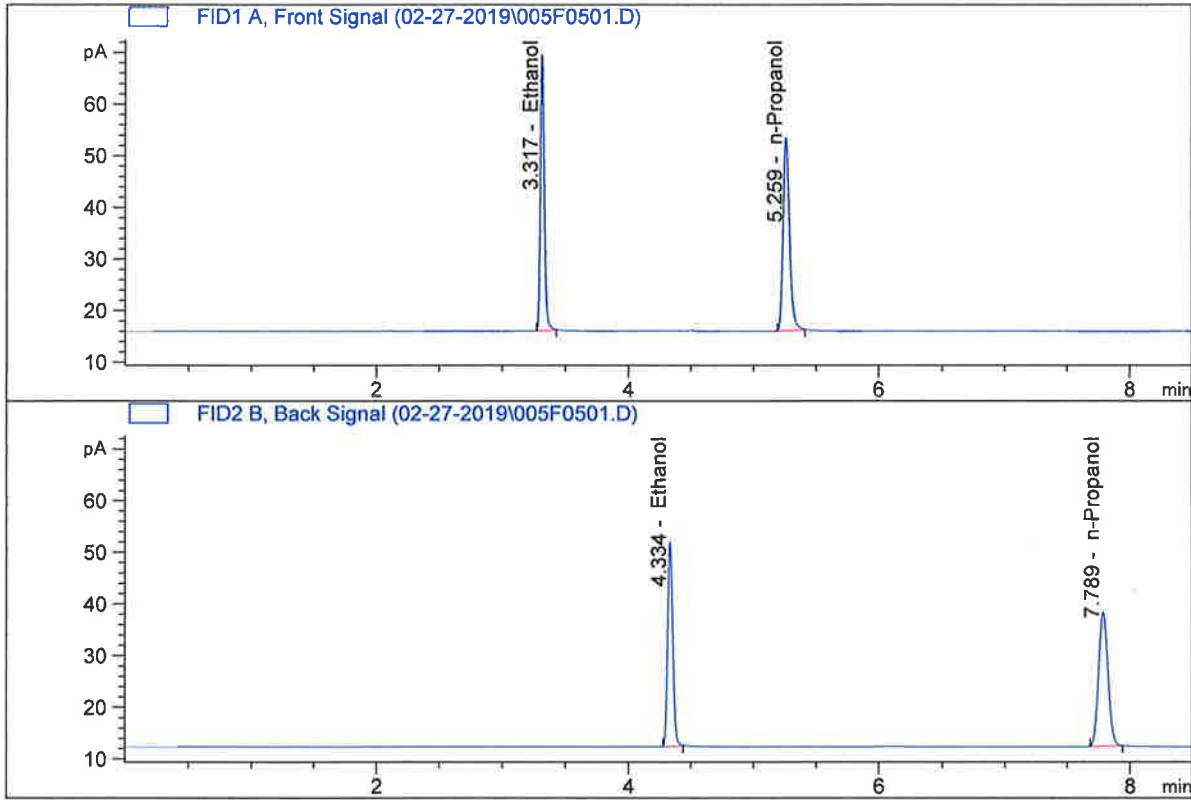


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	117.86619	0.5027	g/100cc
2.	Ethanol	Column 2:	115.28214	0.5032	g/100cc
3.	n-Propanol	Column 1:	135.46065	1.0000	g/100cc
4.	n-Propanol	Column 2:	135.41518	1.0000	g/100cc

RC

ISP Forensic Services Blood Alcohol Report

Sample Name : ISTD BLANK-1
 Laboratory : Pocatello
 Injection Date : Feb 27, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN10742043-IT00741010

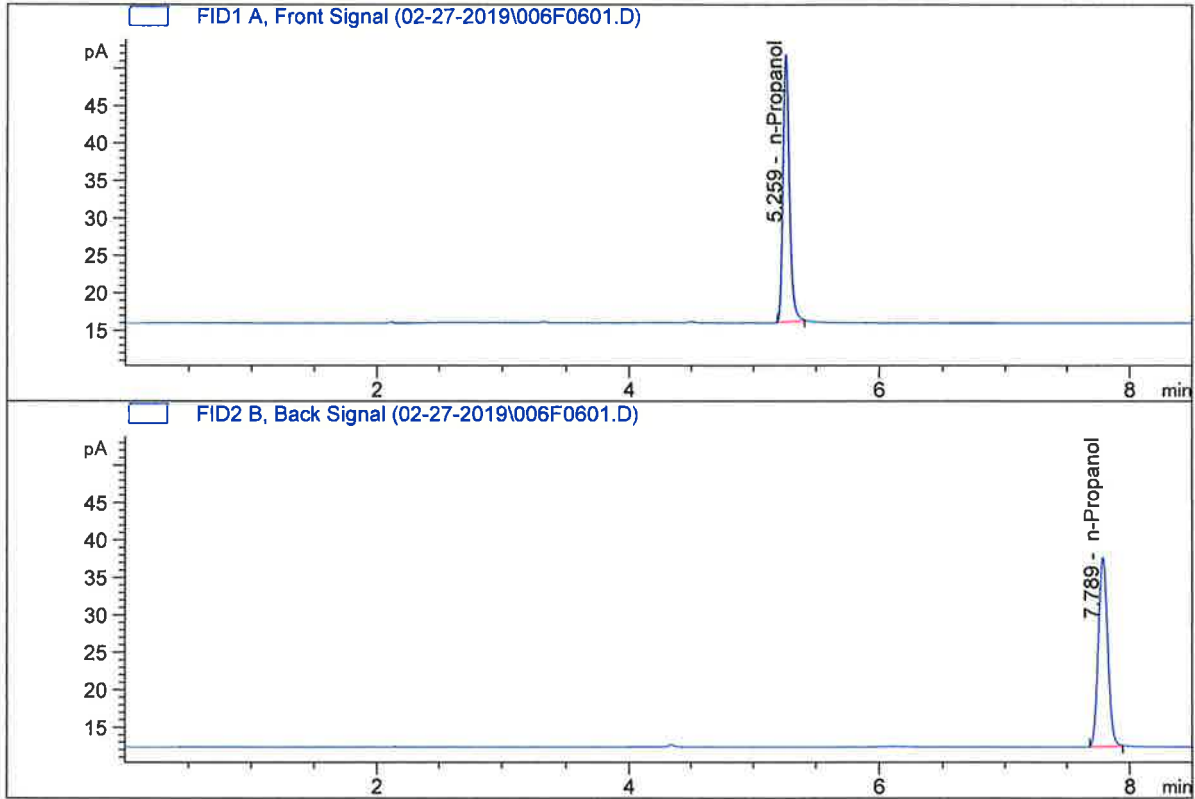

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	129.69971	1.0000	g/100cc
4.	n-Propanol	Column 2:	132.12325	1.0000	g/100cc

Handwritten signature

S a m p l e S u m m a r y


Sequence table: C:\Chem32\1\TEMP\AESEQ\QS_27.02.2019_11.45.30\MASTERCAL.S
Data directory path: C:\Chem32\1\Data\02-27-2019
Logbook: C:\Chem32\1\Data\02-27-2019\MASTERCAL.LOG
Sequence start: 2/27/2019 11:59:16 AM
Sequence Operator: SYSTEM
Operator: SYSTEM

Method file name: C:\CHEM32\1\METHODS\ALCOHOL.M

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #	# Cmp
1	1	1	0.05	-	1.0000	001F0101.D	*	4
2	2	1	0.10	-	1.0000	002F0201.D	*	4
3	3	1	0.20	-	1.0000	003F0301.D	*	4
4	4	1	0.300	-	1.0000	004F0401.D	*	4
5	5	1	0.50	-	1.0000	005F0501.D	*	4
6	6	1	ISTD BLANK-1	-	1.0000	006F0601.D		2

ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STD BLK
 Laboratory : Pocatello
 Injection Date : Mar 7, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN10742043-IT00741010

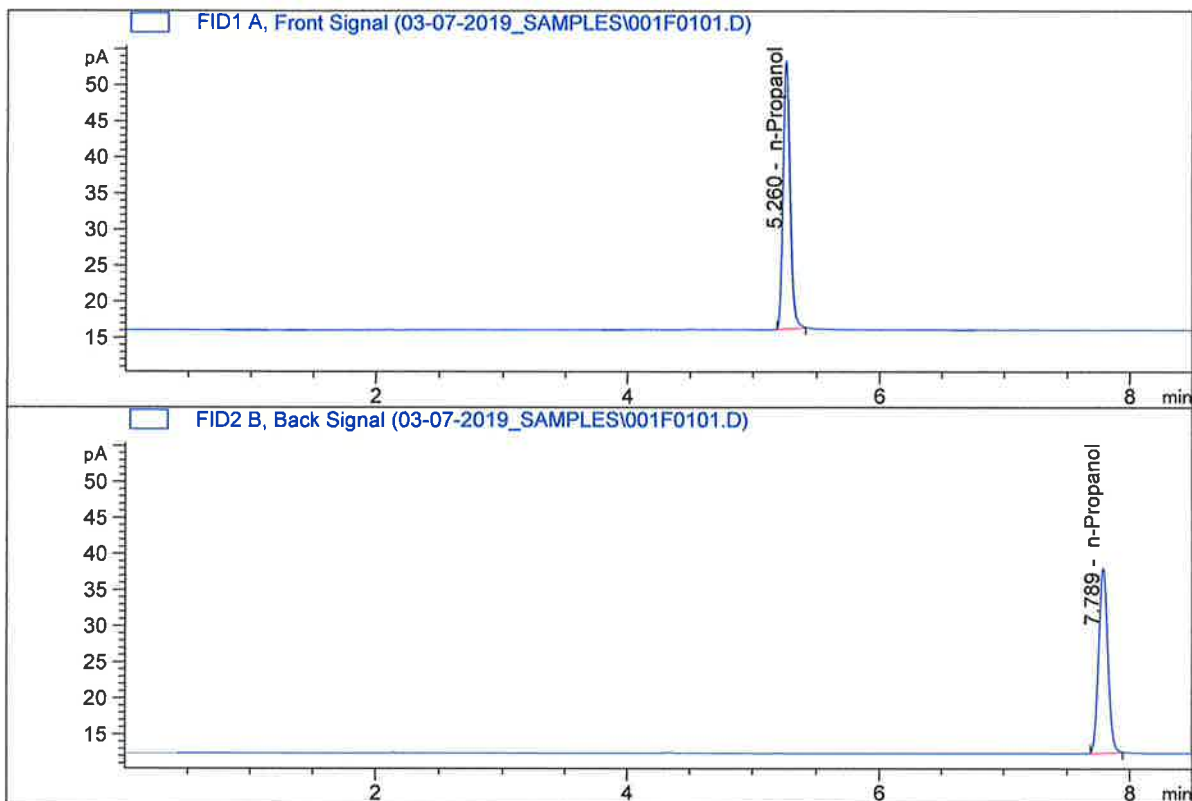


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	138.67451	1.0000	g/100cc
4.	n-Propanol	Column 2:	133.69388	1.0000	g/100cc

RC

ISP Forensic Services Blood Alcohol Report

Sample Name : MULTI-COMP MIX
 Laboratory : Pocatello
 Injection Date : Mar 7, 2019
 Method : ALCOHOL.M
 Acq. Instrument : CN10742043-IT00741010

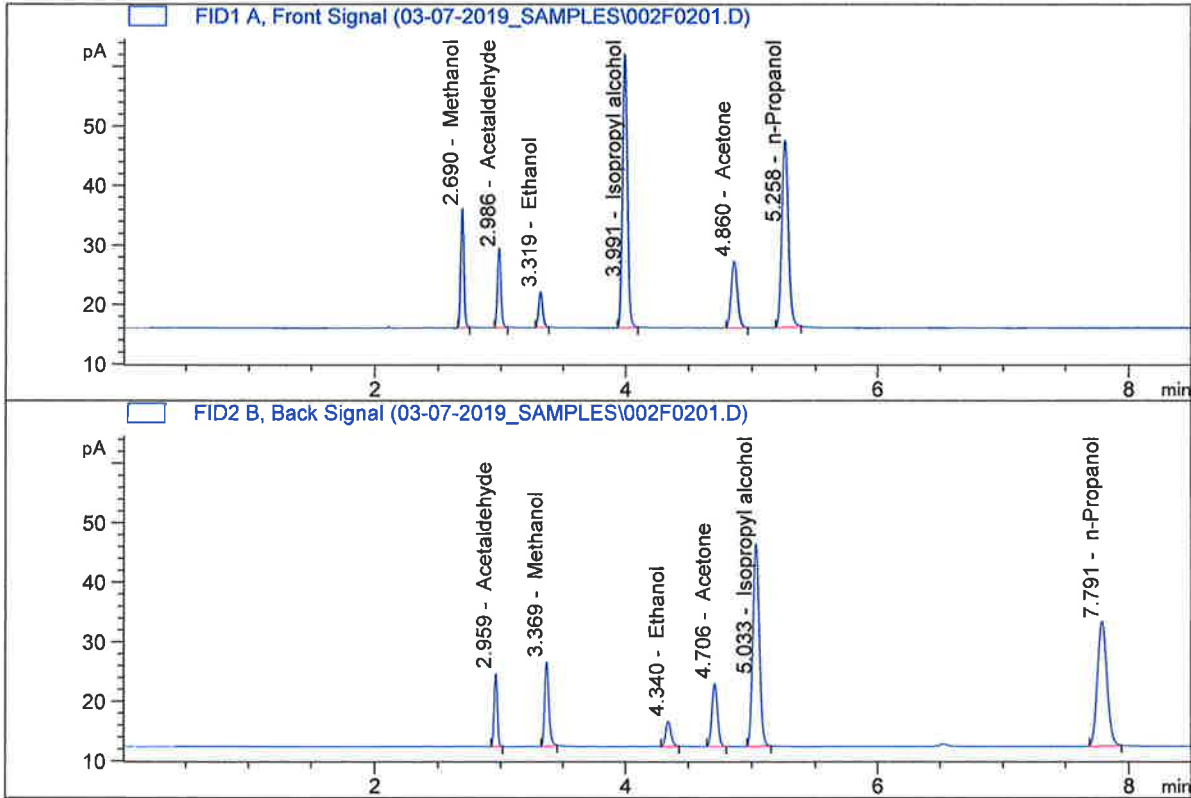


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	13.34820	0.0682	g/100cc
2.	Ethanol	Column 2:	12.68210	0.0683	g/100cc
3.	n-Propanol	Column 1:	113.03785	1.0000	g/100cc
4.	n-Propanol	Column 2:	109.69781	1.0000	g/100cc

HC

ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STD
 Laboratory : Pocatello
 Injection Date : Mar 7, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN10742043-IT00741010

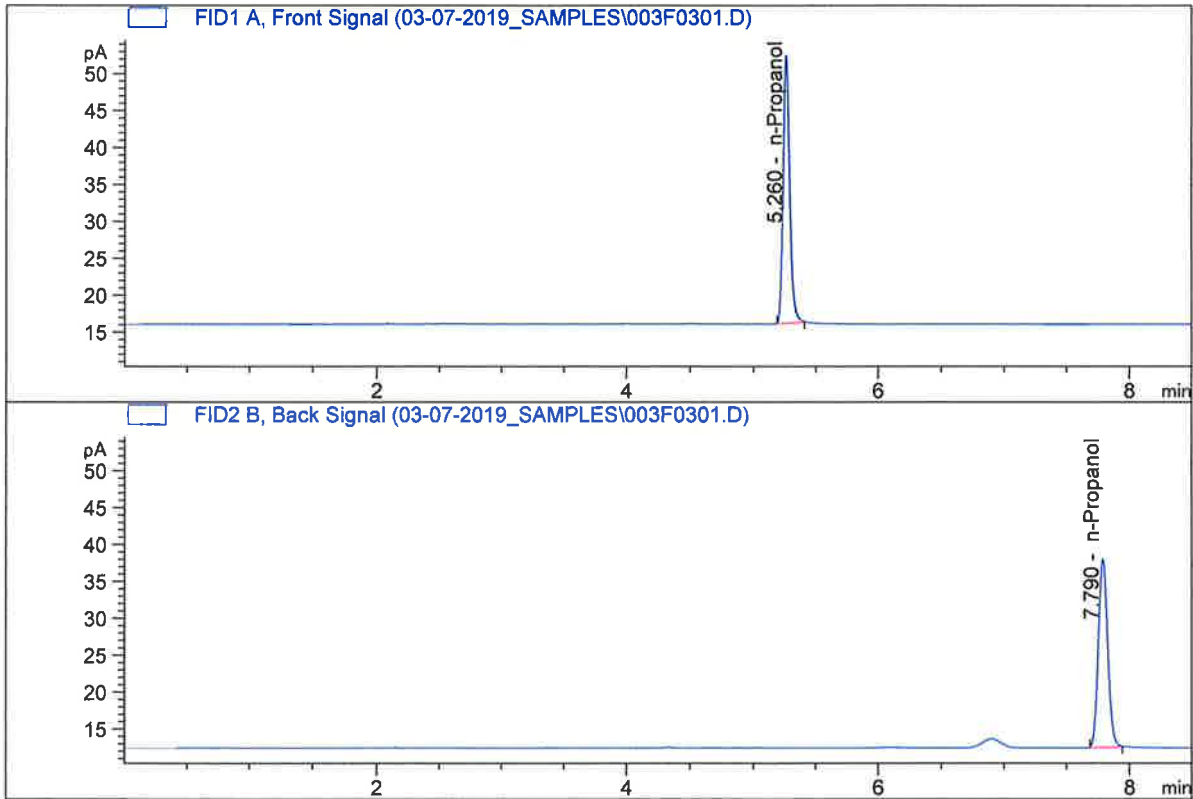

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	134.05920	1.0000	g/100cc
4.	n-Propanol	Column 2:	133.68665	1.0000	g/100cc

Handwritten signature/initials

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC1-1

Analysis Date(s): 07 Mar 2019

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean
Sample Results	0.0770	0.0754	0.0016	0.0762	0.0762
(g/100cc)	0.0772	0.0754	0.0018	0.0763	

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: Alcohol.m
Hamilton Auto-Dilutor Serial Number: ML600HC11379

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.076	0.072	0.080	0.004

Reported Result	
0.076	

Calibration and control data are stored centrally.



Revision: 1

Issue Date: 01/04/2019

Issuing Authority: Quality Manager

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-1-A
 Laboratory : Pocatello
 Injection Date : Mar 7, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN10742043-IT00741010

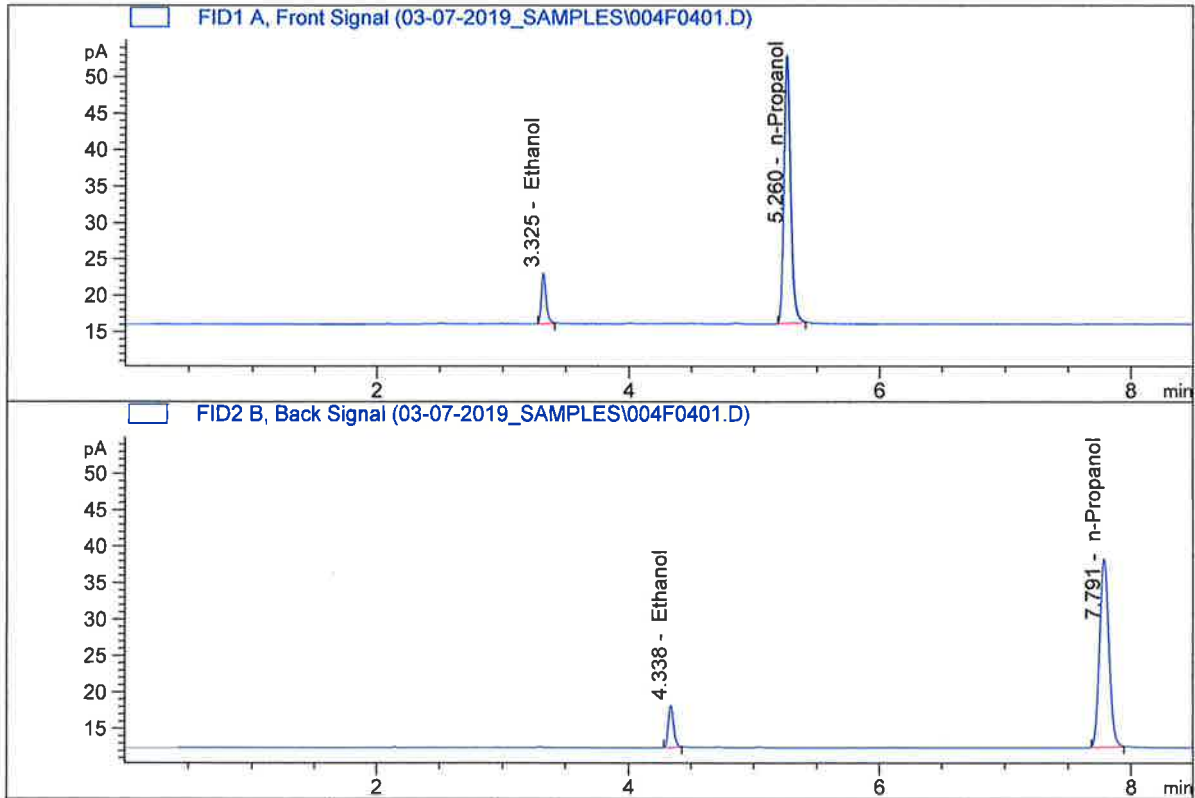


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	18.00385	0.0770	g/100cc
2.	Ethanol	Column 2:	17.20595	0.0754	g/100cc
3.	n-Propanol	Column 1:	135.11807	1.0000	g/100cc
4.	n-Propanol	Column 2:	134.87175	1.0000	g/100cc

JRC

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-1-B
 Laboratory : Pocatello
 Injection Date : Mar 7, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN10742043-IT00741010

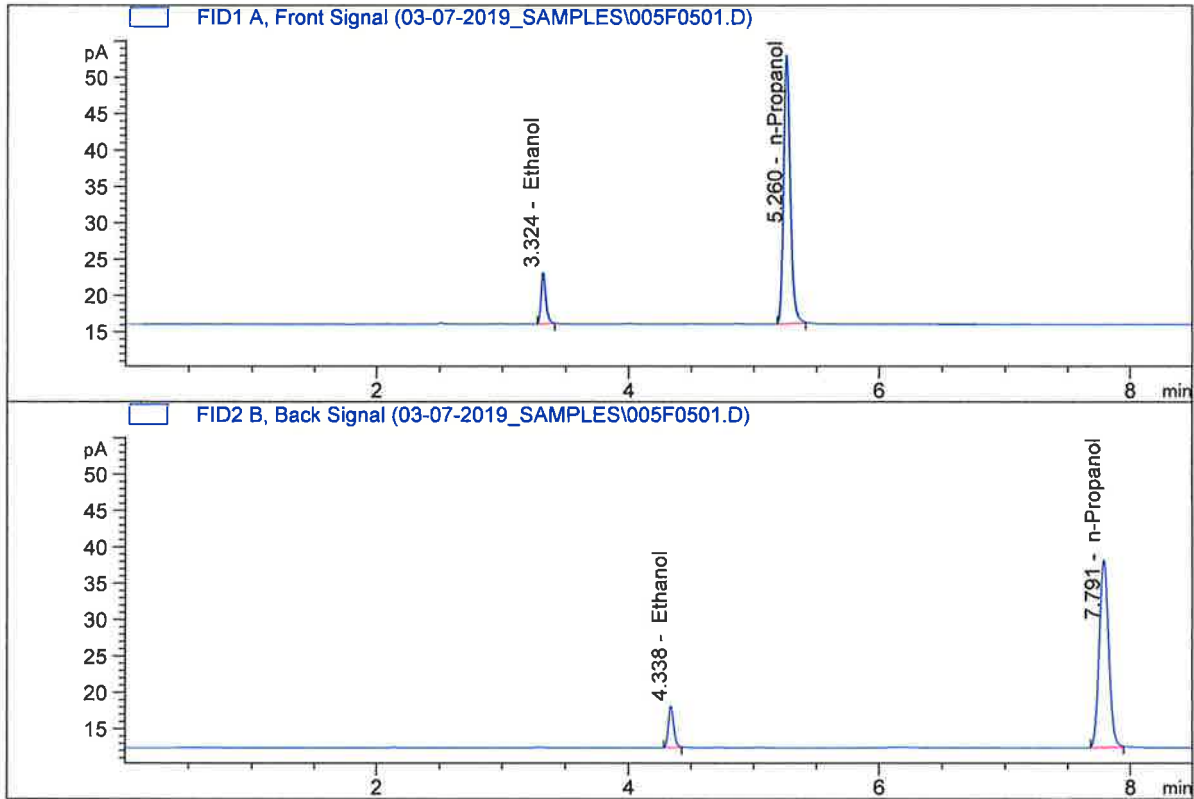

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	18.08614	0.0772	g/100cc
2.	Ethanol	Column 2:	17.17397	0.0754	g/100cc
3.	n-Propanol	Column 1:	135.32729	1.0000	g/100cc
4.	n-Propanol	Column 2:	134.68315	1.0000	g/100cc

Handwritten signature

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: 08 QA

Analysis Date(s): 07 Mar 2019

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean
Sample Results	0.0790	0.0771	0.0019	0.0780	0.0776
(g/100cc)	0.0780	0.0766	0.0014	0.0773	

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: Alcohol.m
Hamilton Auto-Dilutor Serial Number: ML600HC11379

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.077	0.073	0.081	0.004

Reported Result
0.077

Calibration and control data are stored centrally.




Revision: 1

Issue Date: 01/04/2019

Issuing Authority: Quality Manager

ISP Forensic Services Blood Alcohol Report

Sample Name : 08 QA-A
 Laboratory : Pocatello
 Injection Date : Mar 7, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN10742043-IT00741010

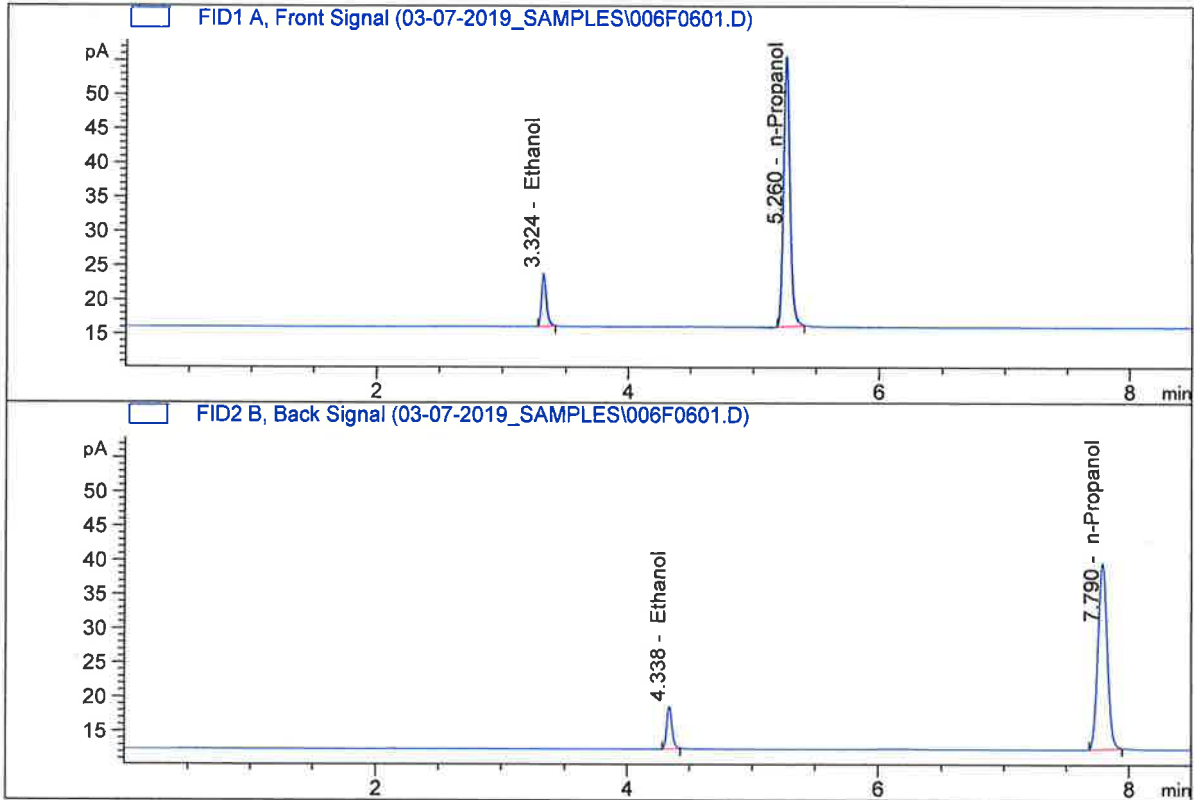


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	19.70754	0.0790	g/100cc
2.	Ethanol	Column 2:	18.60001	0.0771	g/100cc
3.	n-Propanol	Column 1:	144.03264	1.0000	g/100cc
4.	n-Propanol	Column 2:	142.54240	1.0000	g/100cc

JHC

ISP Forensic Services Blood Alcohol Report

Sample Name : 08 QA-B
 Laboratory : Pocatello
 Injection Date : Mar 7, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN10742043-IT00741010

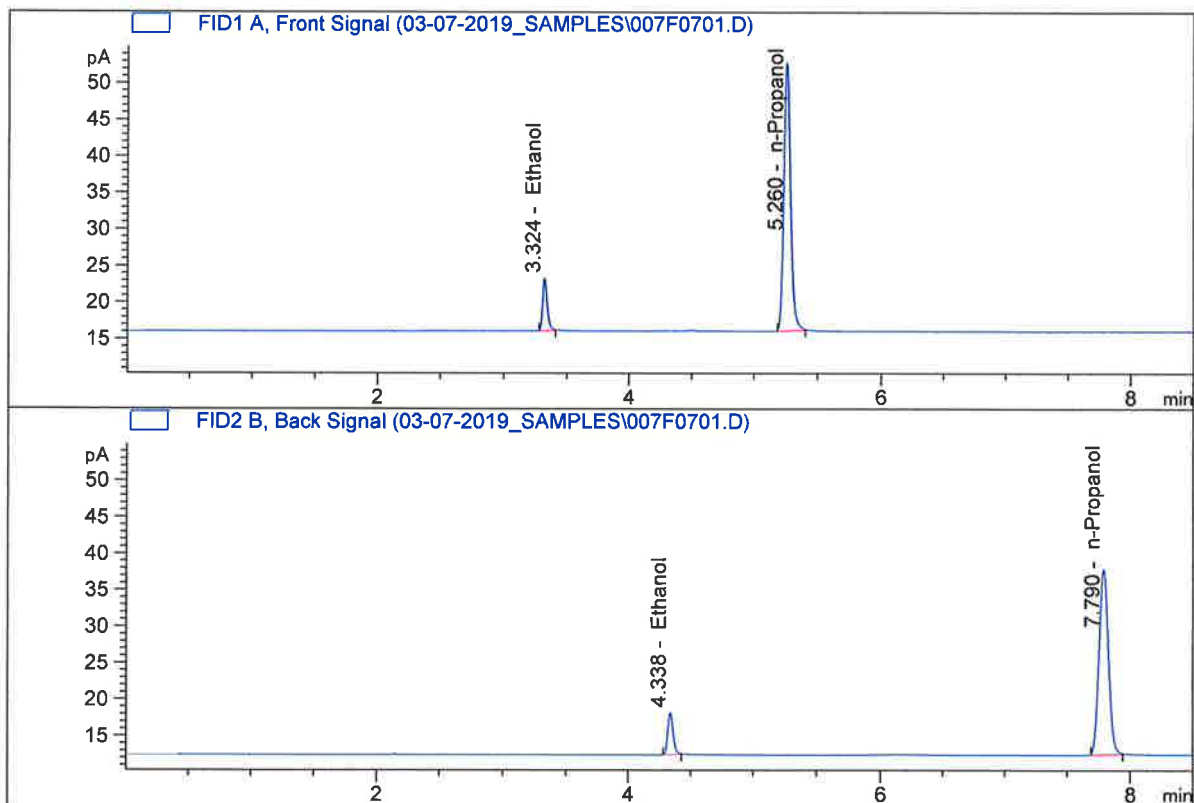

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	18.10993	0.0780	g/100cc
2.	Ethanol	Column 2:	17.16935	0.0766	g/100cc
3.	n-Propanol	Column 1:	134.15504	1.0000	g/100cc
4.	n-Propanol	Column 2:	132.44856	1.0000	g/100cc

AC

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC2-1

Analysis Date(s): 07 Mar 2019

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean
Sample Results	0.1955	0.1950	0.0005	0.1952	0.1960
(g/100cc)	0.1971	0.1965	0.0006	0.1968	

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: Alcohol.m
Hamilton Auto-Dilutor Serial Number: ML600HC11379

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.196	0.186	0.206	0.010

Reported Result	
0.196	

Calibration and control data are stored centrally.




Revision: 1

Issue Date: 01/04/2019

Issuing Authority: Quality Manager

ISP Forensic Services Blood Alcohol Report

Sample Name : QC2-1-A
 Laboratory : Pocatello
 Injection Date : Mar 7, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN10742043-IT00741010

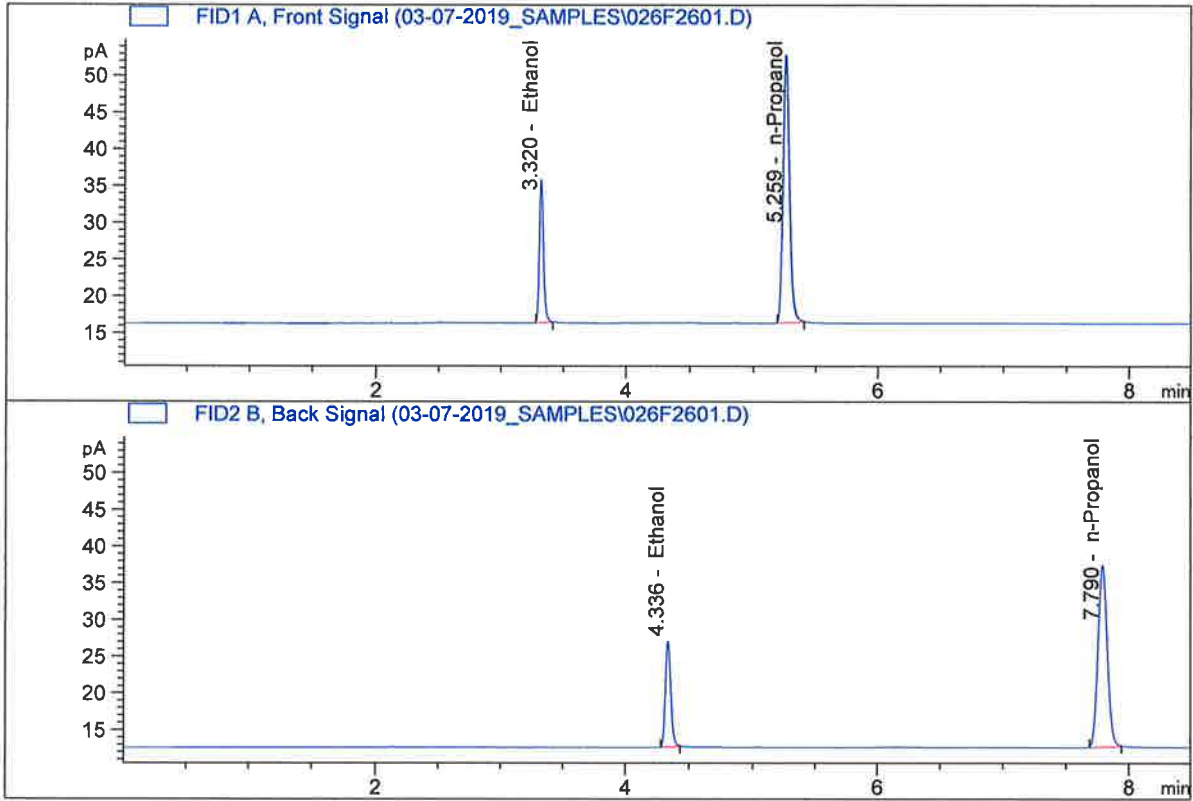


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	44.75013	0.1955	g/100cc
2.	Ethanol	Column 2:	42.62984	0.1950	g/100cc
3.	n-Propanol	Column 1:	132.26707	1.0000	g/100cc
4.	n-Propanol	Column 2:	129.25932	1.0000	g/100cc

RC

ISP Forensic Services Blood Alcohol Report

Sample Name : QC2-1-B
 Laboratory : Pocatello
 Injection Date : Mar 7, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN10742043-IT00741010

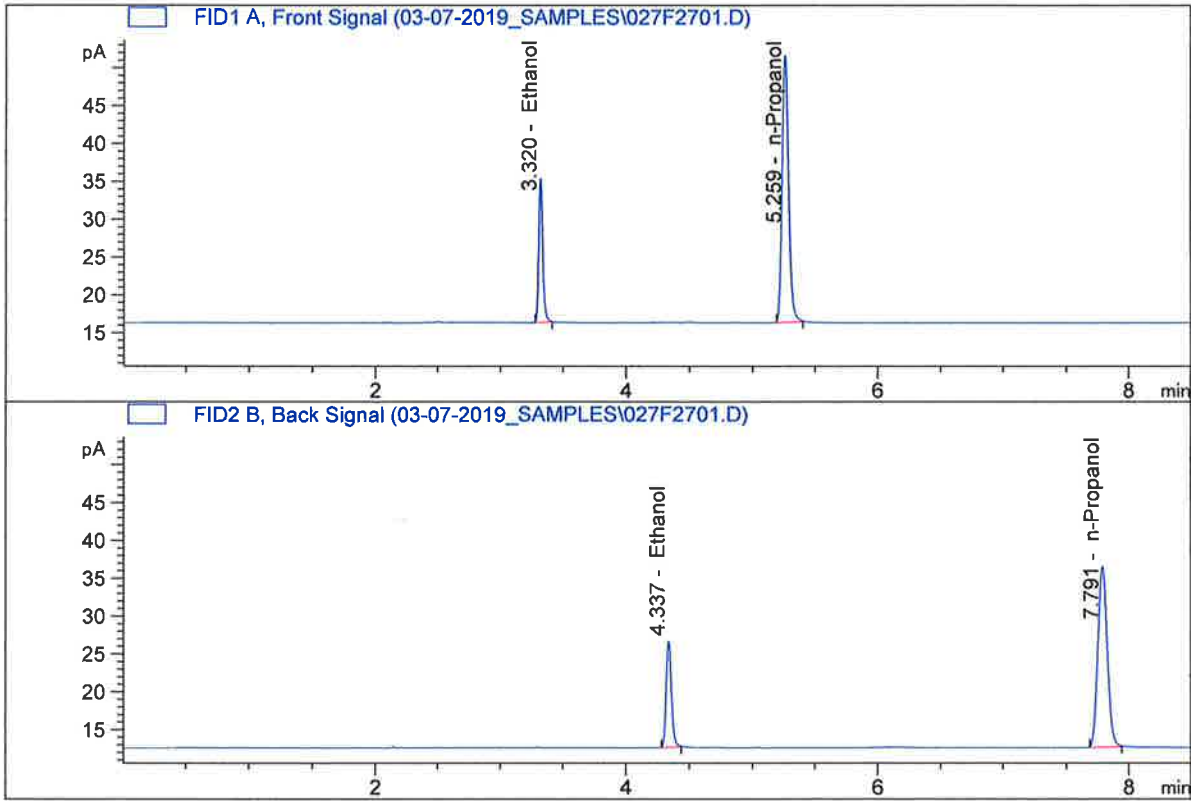

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	43.56390	0.1971	g/100cc
2.	Ethanol	Column 2:	41.54699	0.1965	g/100cc
3.	n-Propanol	Column 1:	127.67390	1.0000	g/100cc
4.	n-Propanol	Column 2:	124.95846	1.0000	g/100cc

RC

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC1-2

Analysis Date(s): 08 Mar 2019

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.0785	0.0771	0.0014	0.0778	0.0781	
(g/100cc)	0.0795	0.0775	0.0020	0.0785		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: Alcohol.m
Hamilton Auto-Dilutor Serial Number: ML600HC11379

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.078	0.074	0.082	0.004

	Reported Result	
	0.078	

Calibration and control data are stored centrally.



Revision: 1

Issue Date: 01/04/2019

Issuing Authority: Quality Manager

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-2-A
 Laboratory : Pocatello
 Injection Date : Mar 8, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN10742043-IT00741010

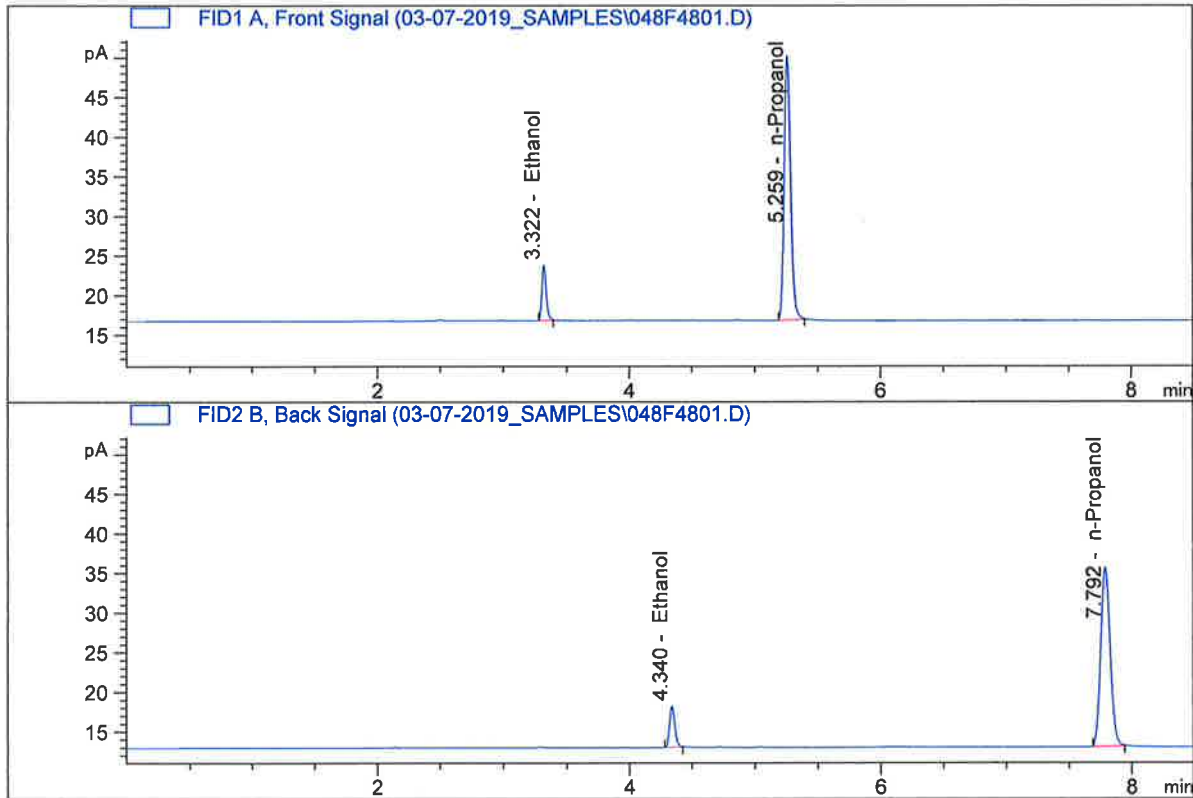


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	16.34459	0.0785	g/100cc
2.	Ethanol	Column 2:	15.43447	0.0771	g/100cc
3.	n-Propanol	Column 1:	120.24786	1.0000	g/100cc
4.	n-Propanol	Column 2:	118.33945	1.0000	g/100cc

RC

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-2-B
 Laboratory : Pocatello
 Injection Date : Mar 8, 2019
 Method : ALCOHOL.M
 Acq. Instrument : CN10742043-IT00741010

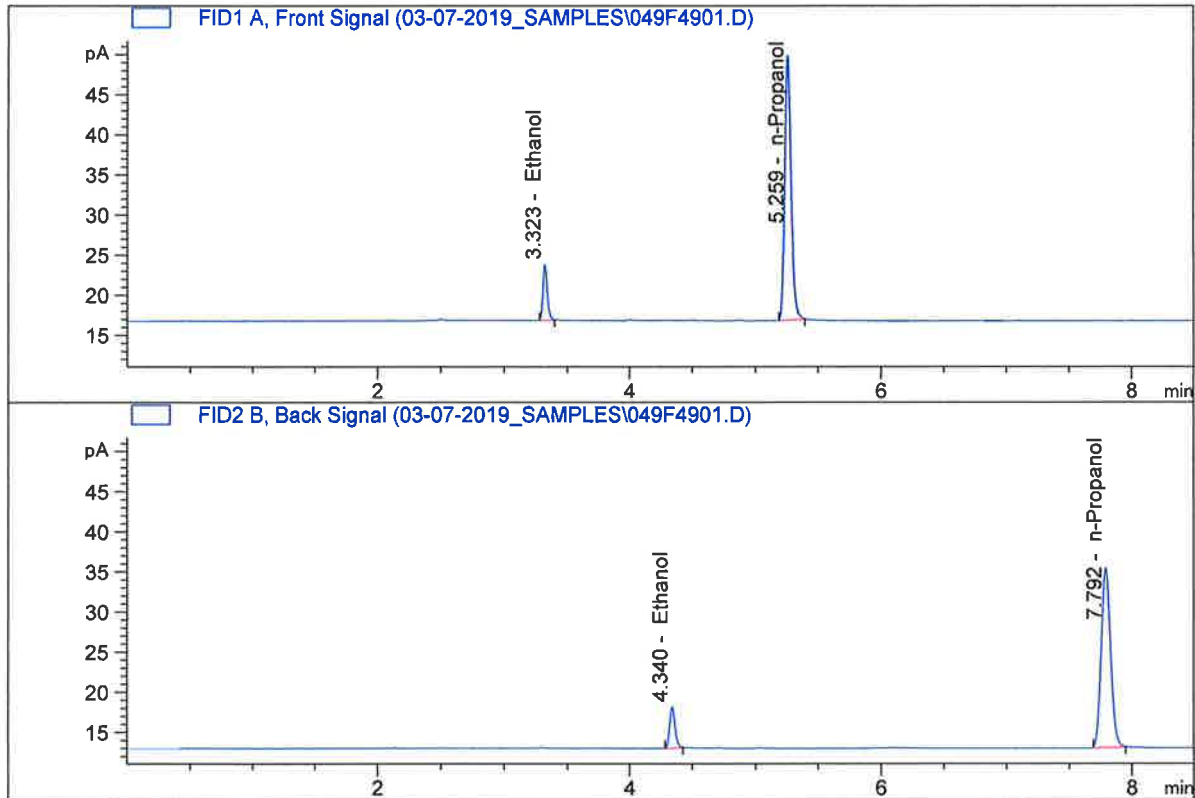

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	16.31587	0.0795	g/100cc
2.	Ethanol	Column 2:	15.32215	0.0775	g/100cc
3.	n-Propanol	Column 1:	118.61121	1.0000	g/100cc
4.	n-Propanol	Column 2:	116.91096	1.0000	g/100cc

RC

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC2-2

Analysis Date(s): 08 Mar 2019

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.2017	0.1999	0.0018	0.2008	0.2012	
(g/100cc)	0.2023	0.2010	0.0013	0.2016		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: Alcohol.m
Hamilton Auto-Dilutor Serial Number: ML600HC11379

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.201	0.190	0.212	0.011

	Reported Result	
	0.201	

Calibration and control data are stored centrally.




Revision: 1

Issue Date: 01/04/2019

Issuing Authority: Quality Manager

ISP Forensic Services Blood Alcohol Report

Sample Name : QC2-2-A
 Laboratory : Pocatello
 Injection Date : Mar 8, 2019
 Method : ALCOHOL.M
 Acq. Instrument : CN10742043-IT00741010

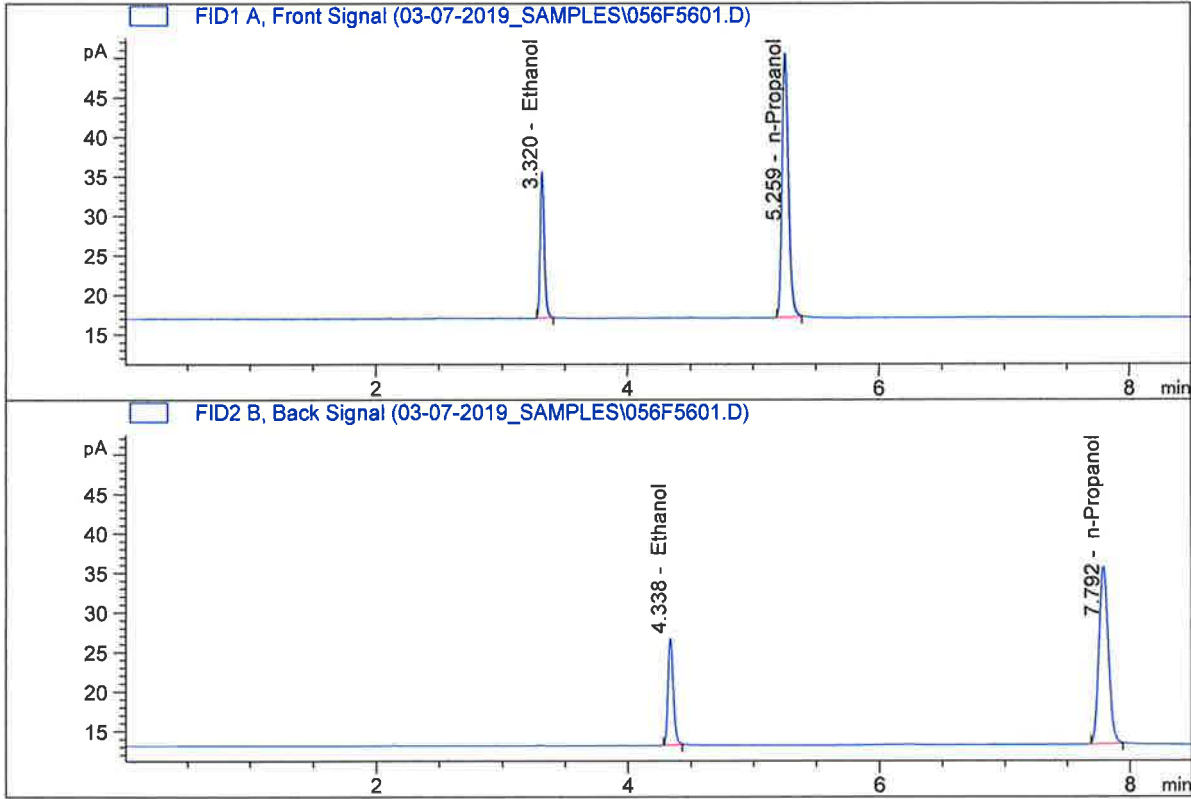


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	41.92079	0.2017	g/100cc
2.	Ethanol	Column 2:	39.78376	0.1999	g/100cc
3.	n-Propanol	Column 1:	120.09132	1.0000	g/100cc
4.	n-Propanol	Column 2:	117.62893	1.0000	g/100cc

HC

ISP Forensic Services Blood Alcohol Report

Sample Name : QC2-2-B
 Laboratory : Pocatello
 Injection Date : Mar 8, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN10742043-IT00741010

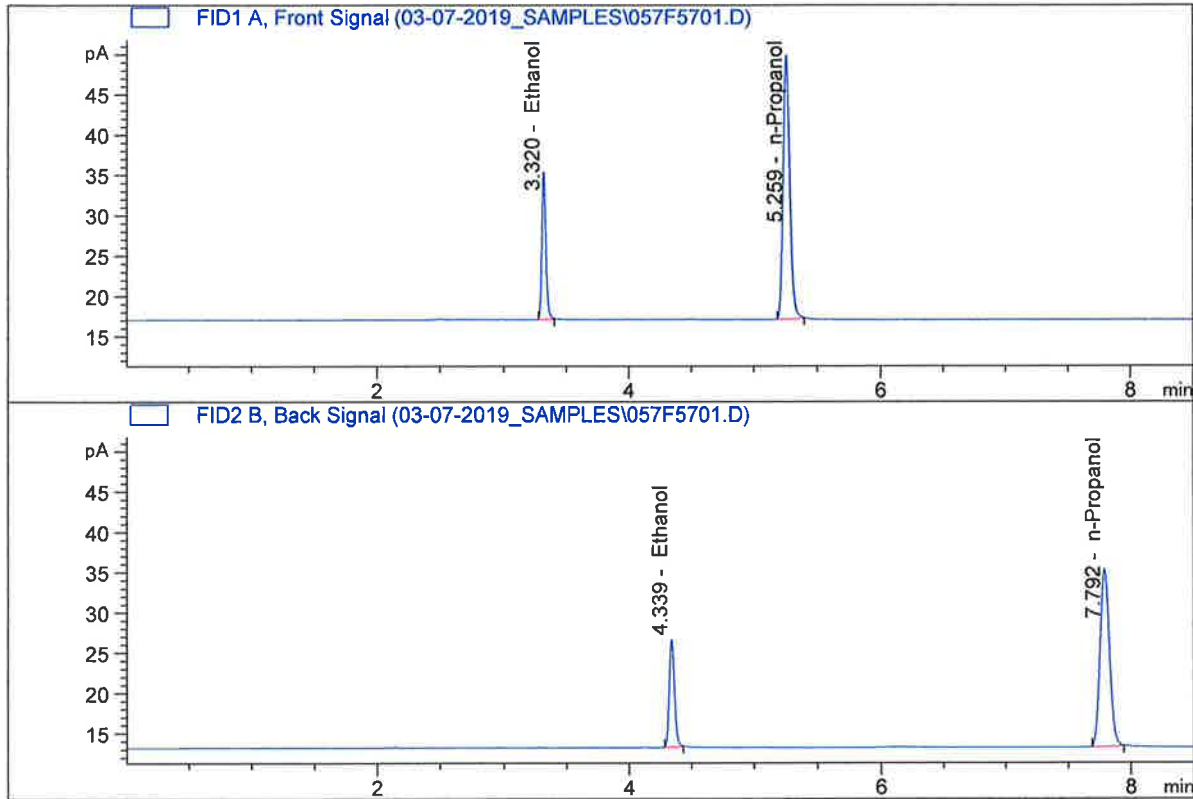


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	41.36036	0.2023	g/100cc
2.	Ethanol	Column 2:	39.25709	0.2010	g/100cc
3.	n-Propanol	Column 1:	118.12123	1.0000	g/100cc
4.	n-Propanol	Column 2:	115.42647	1.0000	g/100cc

Handwritten signature/initials

ISP Forensic Services Blood Alcohol Report

Sample Name : INT STD BLK
 Laboratory : Pocatello
 Injection Date : Mar 8, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN10742043-IT00741010

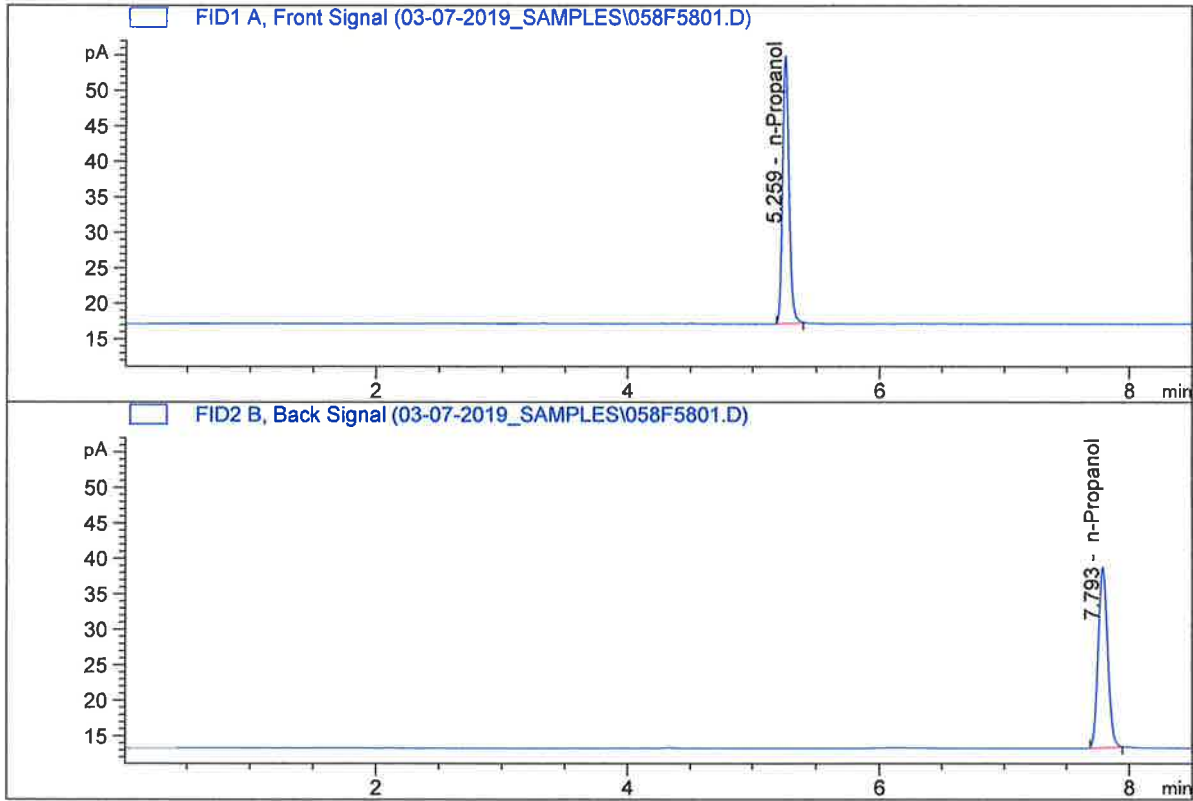

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	135.08937	1.0000	g/100cc
4.	n-Propanol	Column 2:	132.70358	1.0000	g/100cc

AC

Sample Summary

Sequence table: C:\Chem32\1\TEMP\AESEQ\QS_07.03.2019_04.54.26\RC03MAR2019.S
 Data directory path: C:\Chem32\1\Data\03-07-2019_SAMPLES
 Logbook: C:\Chem32\1\Data\03-07-2019_SAMPLES\RC03MAR2019.LOG
 Sequence start: 3/7/2019 5:08:15 PM
 Sequence Operator: SYSTEM
 Operator: SYSTEM

Method file name: C:\CHEM32\1\METHODS\ALCOHOL.M

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #	# Cmp
1	1	1	INTERNAL STD BLK	-	1.0000	001F0101.D		2
2	2	1	MULTI-COMP MIX	-	1.0000	002F0201.D		12
3	3	1	INTERNAL STD	-	1.0000	003F0301.D		2
4	4	1	QC1-1-A	-	1.0000	004F0401.D		4
5	5	1	QC1-1-B	-	1.0000	005F0501.D		4
6	6	1	08 QA-A	-	1.0000	006F0601.D		4
7	7	1	08 QA-B	-	1.0000	007F0701.D		4
8	8	1	P2019-0625-1-A	-	1.0000	008F0801.D		4
9	9	1	P2019-0625-1-B	-	1.0000	009F0901.D		4
10	10	1	M2019-0626-1-A	-	1.0000	010F1001.D		2
11	11	1	M2019-0626-1-B	-	1.0000	011F1101.D		2
12	12	1	P2019-0627-1-A	-	1.0000	012F1201.D		6
13	13	1	P2019-0627-1-B	-	1.0000	013F1301.D		6
14	14	1	P2019-0632-1-A	-	1.0000	014F1401.D		4
15	15	1	P2019-0632-1-B	-	1.0000	015F1501.D		4
16	16	1	P2019-0645-1-A	-	1.0000	016F1601.D		4
17	17	1	P2019-0645-1-B	-	1.0000	017F1701.D		4
18	18	1	P2019-0657-1-A	-	1.0000	018F1801.D		6
19	19	1	P2019-0657-1-B	-	1.0000	019F1901.D		6
20	20	1	P2019-0664-1-A	-	1.0000	020F2001.D		4
21	21	1	P2019-0664-1-B	-	1.0000	021F2101.D		4
22	22	1	P2019-0665-1-A	-	1.0000	022F2201.D		4
23	23	1	P2019-0665-1-B	-	1.0000	023F2301.D		4
24	24	1	P2019-0668-2-A	-	1.0000	024F2401.D		5
25	25	1	P2019-0668-2-B	-	1.0000	025F2501.D		4
26	26	1	QC2-1-A	-	1.0000	026F2601.D		4
27	27	1	QC2-1-B	-	1.0000	027F2701.D		4
28	28	1	P2019-0671-1-A	-	1.0000	028F2801.D		6
29	29	1	P2019-0671-1-B	-	1.0000	029F2901.D		6
30	30	1	P2019-0672-1-A	-	1.0000	030F3001.D		6
31	31	1	P2019-0672-1-B	-	1.0000	031F3101.D		6
32	32	1	P2019-0673-1-A	-	1.0000	032F3201.D		6
33	33	1	P2019-0673-1-B	-	1.0000	033F3301.D		6
34	34	1	P2019-0674-1-A	-	1.0000	034F3401.D		5
35	35	1	P2019-0674-1-B	-	1.0000	035F3501.D		6
36	36	1	P2019-0685-1-A	-	1.0000	036F3601.D		4
37	37	1	P2019-0685-1-B	-	1.0000	037F3701.D		4
38	38	1	P2019-0686-1-A	-	1.0000	038F3801.D		4
39	39	1	P2019-0686-1-B	-	1.0000	039F3901.D		4
40	40	1	P2019-0707-1-A	-	1.0000	040F4001.D		2
41	41	1	P2019-0707-1-B	-	1.0000	041F4101.D		2
42	42	1	P2019-0708-1-A	-	1.0000	042F4201.D		4
43	43	1	P2019-0708-1-B	-	1.0000	043F4301.D		4
44	44	1	P2019-0709-1-A	-	1.0000	044F4401.D		4
45	45	1	P2019-0709-1-B	-	1.0000	045F4501.D		4
46	46	1	P2019-0736-1-A	-	1.0000	046F4601.D		2

Run #	Location	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #	# Cmp
47	47	1	P2019-0736-1-B	-	1.0000	047F4701.D		2
48	48	1	QC1-2-A	-	1.0000	048F4801.D		4
49	49	1	QC1-2-B	-	1.0000	049F4901.D		4
50	50	1	P2019-0737-1-A	-	1.0000	050F5001.D		2
51	51	1	P2019-0737-1-B	-	1.0000	051F5101.D		2
52	52	1	P2019-0737-2-A	-	1.0000	052F5201.D		2
53	53	1	P2019-0737-2-B	-	1.0000	053F5301.D		2
54	54	1	M2019-0876-4-A	-	1.0000	054F5401.D		4
55	55	1	M2019-0876-4-B	-	1.0000	055F5501.D		4
56	56	1	QC2-2-A	-	1.0000	056F5601.D		4
57	57	1	QC2-2-B	-	1.0000	057F5701.D		4
58	58	1	INT STD BLK	-	1.0000	058F5801.D		2

RC