

Quantitative Analysis for Ethanol & Qualitative Analysis for Other Volatiles

Analytical Method(s): 1.0

Device: Hamilton MICROLAB 600A Liquid Processor/Dilutor Serial Number: ML600HC11378

Volatiles Quality Assurance Controls Run Date(s): 5/16/19

Calibration Date: 5/9/18

Control level	Expiration	Lot #	Target Value	Acceptable Range	Overall Results
Level 1	Jan-22	1801036	0.0812	0.0731-0.0893	0.0799 g/100cc
					0.0851 g/100cc
Level 2	Mar-22	1803028	0.2035	0.1832-0.2238	0.2042 g/100cc
					g/100cc
Multi-Component mixture:			Curve Fit:	Lot #	ok
			Column 1	0.99998	0.99996
			Column 2		

Ethanol Calibration Reference Material

Calibrator level	Target Value	Acceptable Range	Column 1	Column 2	Precision	Mean
50	0.050	0.045 - 0.055	0.0506	0.0522	0.0016	0.0514
100	0.100	0.090 - 0.110	0.0992	0.0991	0.0001	0.0991
200	0.200	0.180 - 0.220	0.1990	0.1980	0.001	0.1985
300	0.300	0.270 - 0.330	0.3017	0.3000	0.0017	0.3008
500	0.500	0.450 - 0.550	0.4995	0.5008	0.0013	0.5001

Aqueous Controls

Control level	Target Value	Acceptable Range	Overall Results
80	0.080	0.076 - 0.084	0.080 g/100cc


REVIEWED
By Melissa (Nikka) Bradley at 3:15 pm, May 17, 2019

NB

ds

Worklist: 3394


<u>LAB CASE</u>	<u>ITEM</u>	<u>TASK ID</u>	<u>DESCRIPTION</u>
M2019-2164	1	152022	Alcohol Analysis
M2019-2174	2	151286	Alcohol Analysis
M2019-2199	1	151376	Alcohol Analysis
M2019-2203	1	151451	Alcohol Analysis
M2019-2224	1	151606	Alcohol Analysis
M2019-2225	1	151607	Alcohol Analysis
M2019-2226	1	151608	Alcohol Analysis
M2019-2227	1	151613	Alcohol Analysis
M2019-2244	1	151662	Alcohol Analysis
M2019-2261	1	151693	Alcohol Analysis
M2019-2262	1	151707	Alcohol Analysis
M2019-2278	1	151782	Alcohol Analysis

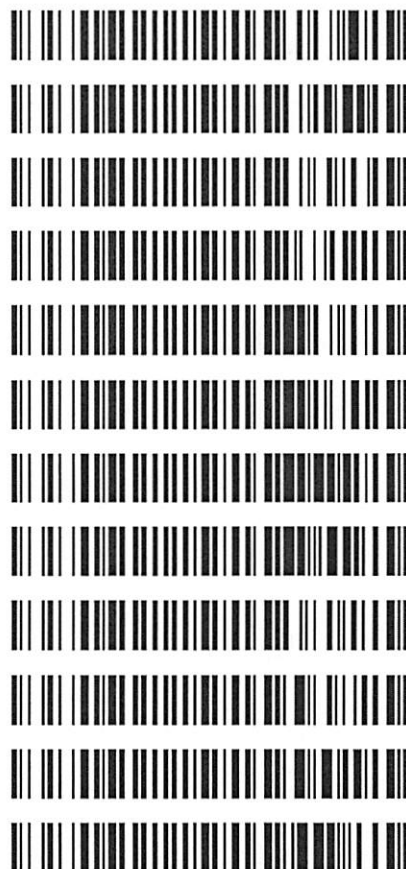

JG

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.050 FN04271601
 Laboratory : Meridian
 Injection Date : May 9, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

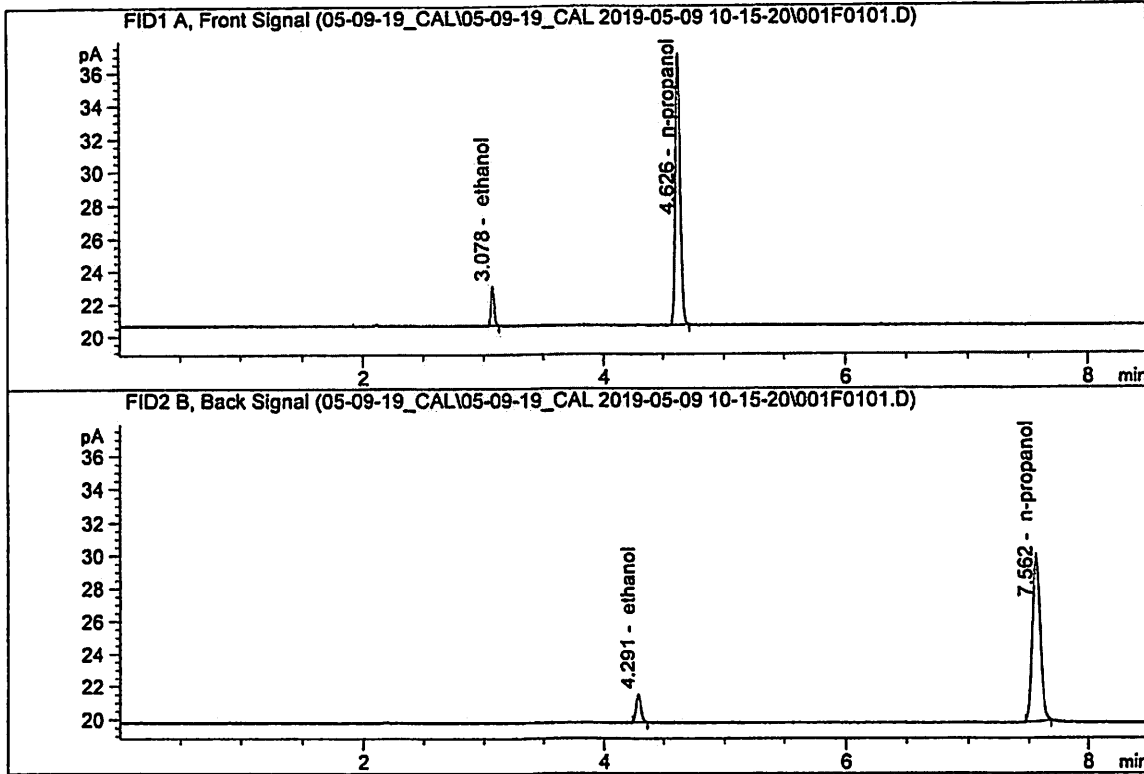


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	4.41218	0.0506	g/100cc
2.	Ethanol	Column 2:	4.58750	0.0522	g/100cc
3.	n-Propanol	Column 1:	46.58786	1.0000	g/100cc
4.	n-Propanol	Column 2:	48.71809	1.0000	g/100cc

dt

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.100 FN08101601
 Laboratory : Meridian
 Injection Date : May 9, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

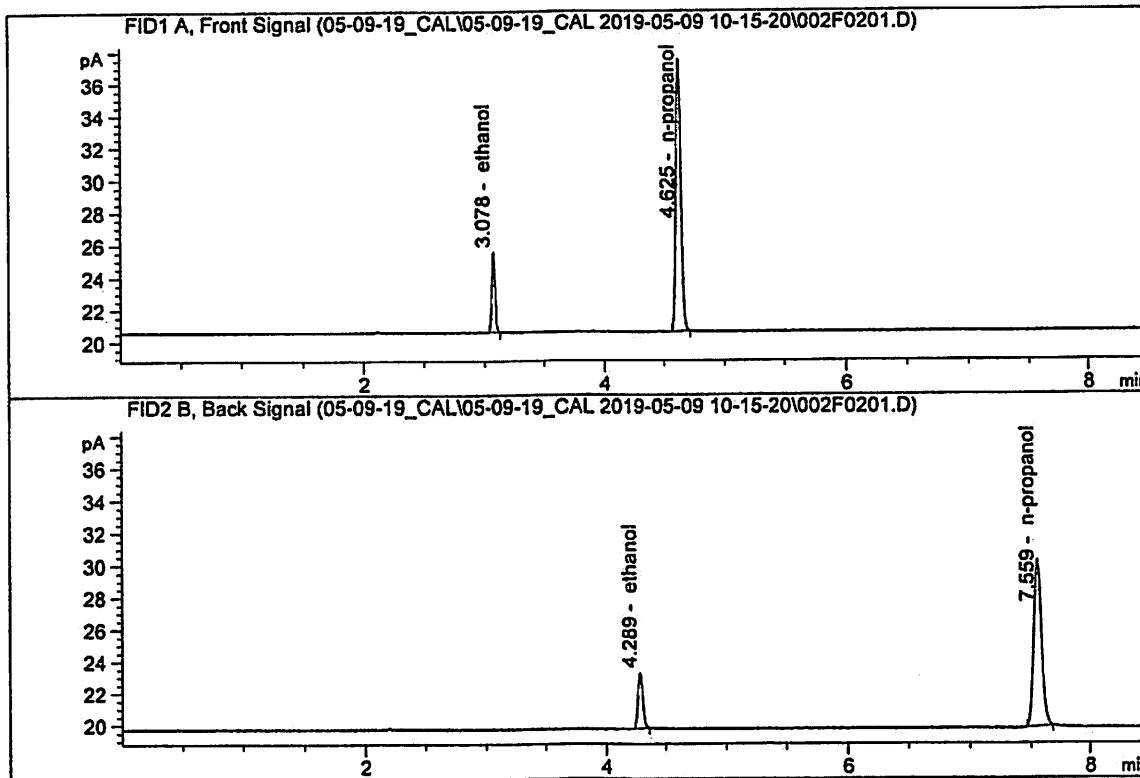


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	8.93847	0.0992	g/100cc
2.	Ethanol	Column 2:	9.24911	0.0991	g/100cc
3.	n-Propanol	Column 1:	47.95212	1.0000	g/100cc
4.	n-Propanol	Column 2:	49.83683	1.0000	g/100cc

2

ISP Forensic Services Blood Alcohol Report


Sample Name : 0.200 FN03301601
 Laboratory : Meridian
 Injection Date : May 9, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

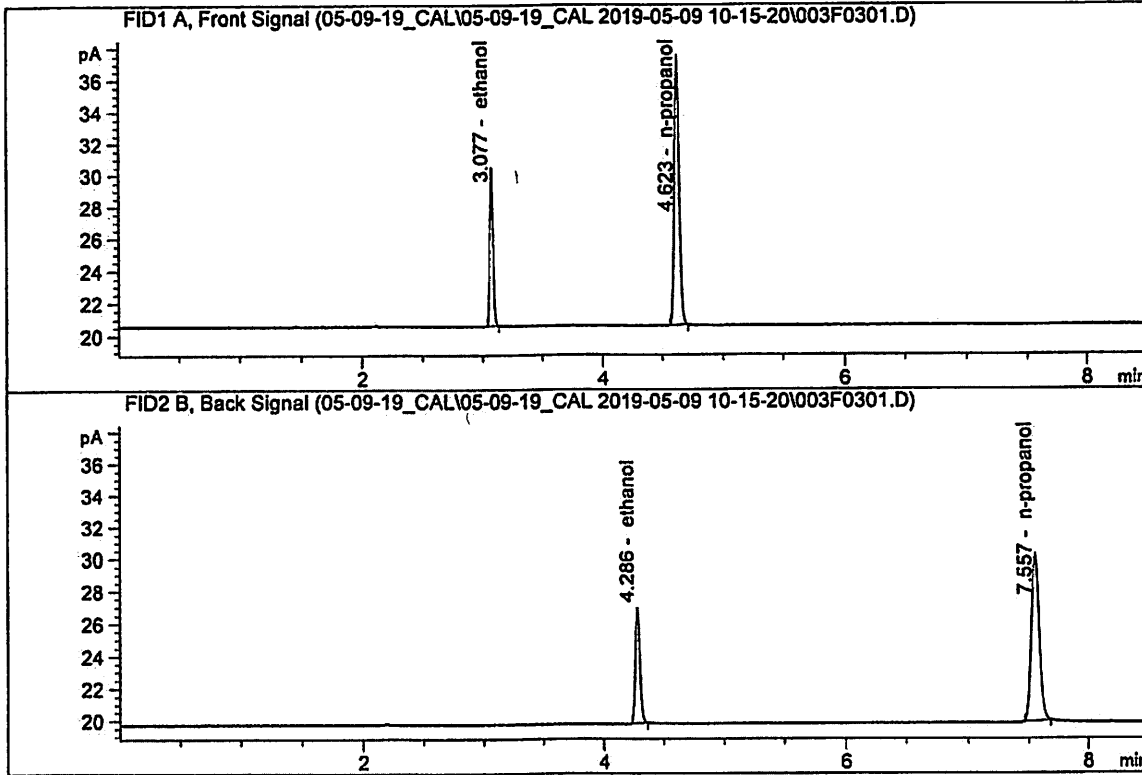

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	18.03616	0.1990	g/100cc
2.	Ethanol	Column 2:	18.85801	0.1980	g/100cc
3.	n-Propanol	Column 1:	48.16090	1.0000	g/100cc
4.	n-Propanol	Column 2:	49.84030	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.300 FN02121601
 Laboratory : Meridian
 Injection Date : May 9, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

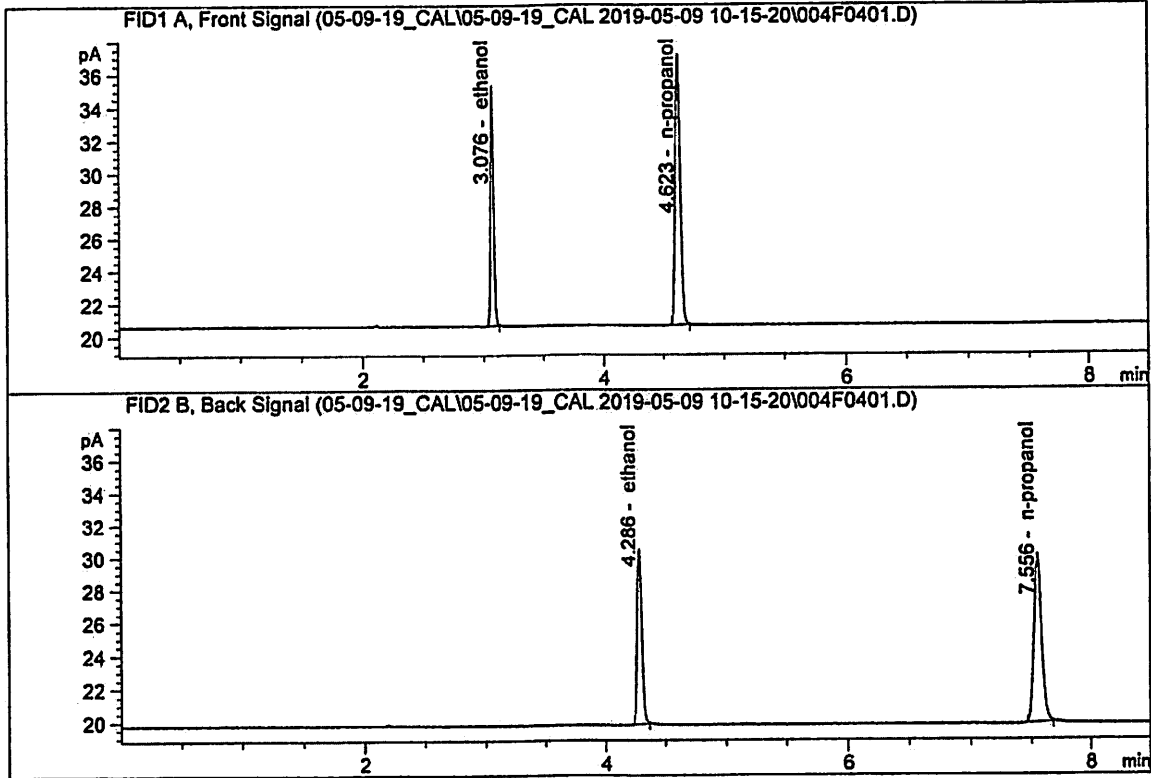


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	26.76689	0.3017	g/100cc
2.	Ethanol	Column 2:	28.08107	0.3000	g/100cc
3.	n-Propanol	Column 1:	47.10820	1.0000	g/100cc
4.	n-Propanol	Column 2:	48.64799	1.0000	g/100cc

JK

ISP Forensic Services Blood Alcohol Report


Sample Name : 0.500 FN08031602
 Laboratory : Meridian
 Injection Date : May 9, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

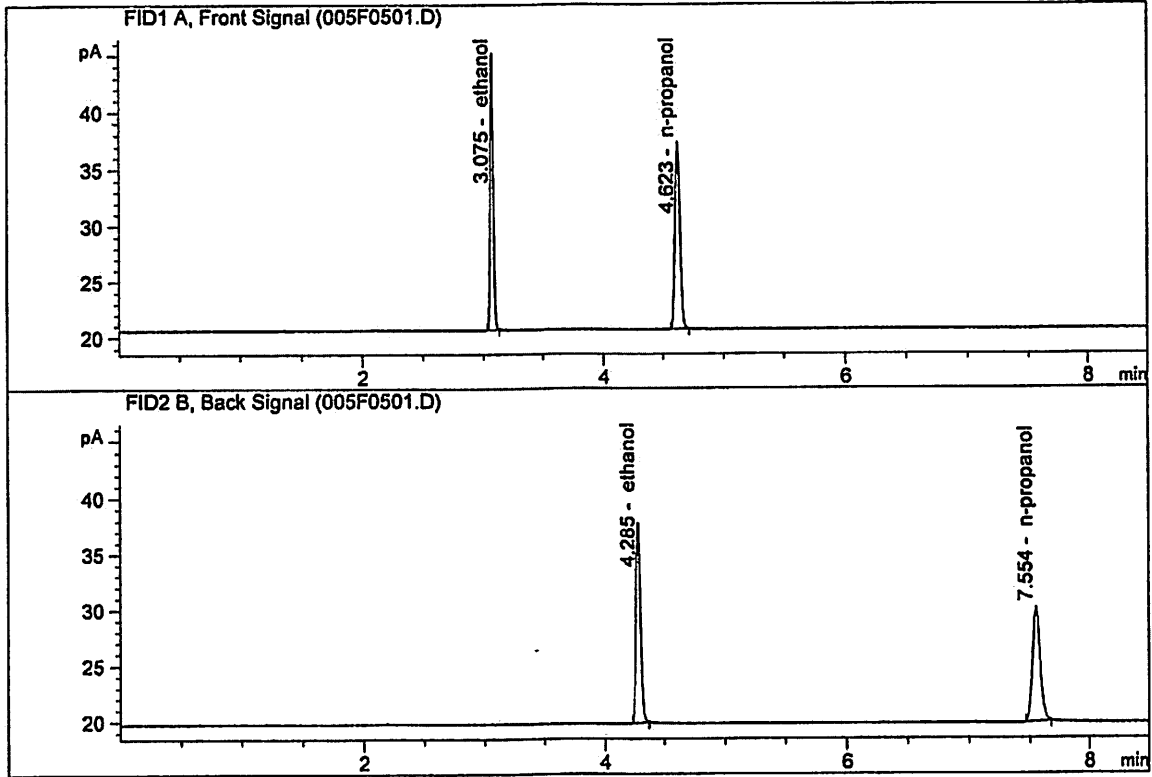

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	44.75016	0.4995	g/100cc
2.	Ethanol	Column 2:	47.43238	0.5008	g/100cc
3.	n-Propanol	Column 1:	47.54111	1.0000	g/100cc
4.	n-Propanol	Column 2:	48.97371	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STANDARD BLANK
 Laboratory : Meridian
 Injection Date : May 9, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

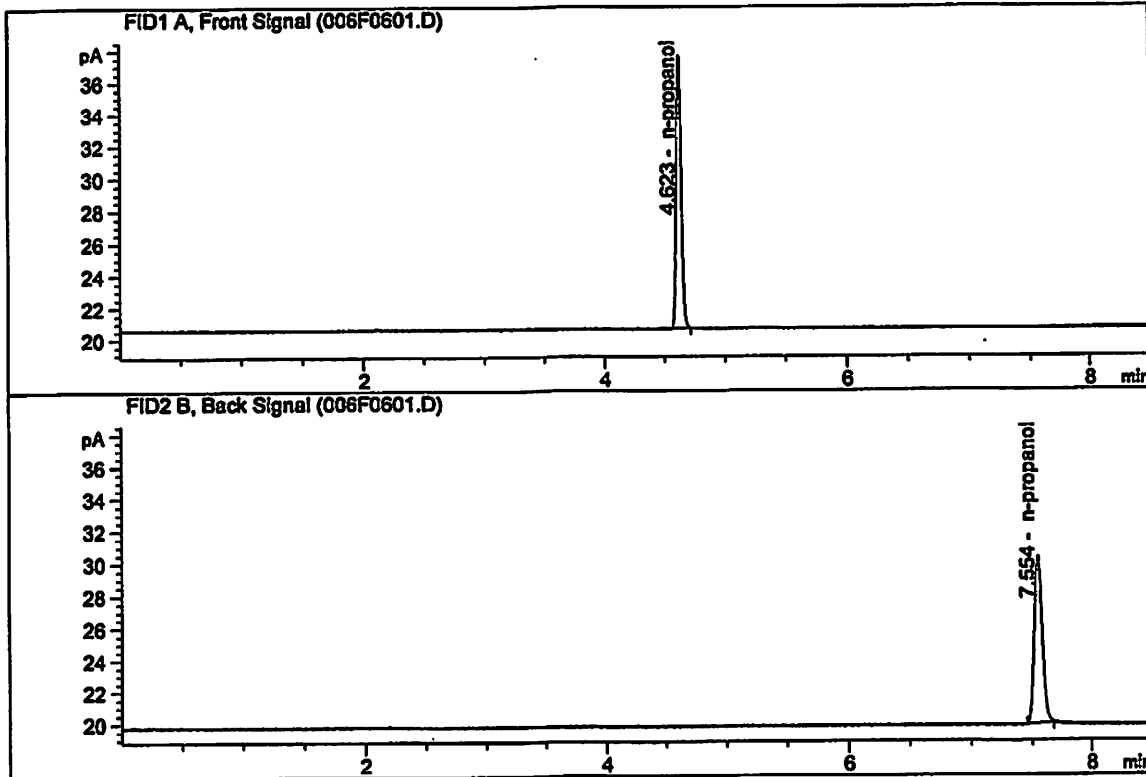

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	48.23984	1.0000	g/100cc
4.	n-Propanol	Column 2:	49.77007	1.0000	g/100cc

JK

S a m p l e S u m m a r y

Sequence table: C:\Chem32\1\Data\05-09-19_CAL\05-09-19_CAL 2019-05-09 10-15-20\05-09-19_CAL.S
 Data directory path: C:\Chem32\1\Data\05-09-19_CAL\05-09-19_CAL 2019-05-09 10-15-20\
 Logbook: C:\Chem32\1\Data\05-09-19_CAL\05-09-19_CAL 2019-05-09 10-15-20\05-09-19_CAL.LOG
 Sequence start: 5/9/2019 10:30:02 AM
 Sequence Operator: SYSTEM
 Operator: SYSTEM

Method file name: C:\Chem32\1\Data\05-09-19_CAL\05-09-19_CAL 2019-05-09 10-15-20\ALCOHOL.M

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #	# Cmp
1	1	1	0.050 FN04271601	-	1.0000	001F0101.D	*	4
2	2	1	0.100 FN08101601	-	1.0000	002F0201.D	*	4
3	3	1	0.200 FN03301601	-	1.0000	003F0301.D	*	4
4	4	1	0.300 FN02121601	-	1.0000	004F0401.D	*	4
5	5	1	0.500 FN08031602	-	1.0000	005F0501.D	*	4
6	6	1	INTERNAL STANDAR	-	1.0000	006F0601.D		2

JK

=====
Calibration Table
=====

General Calibration Setting

Calib. Data Modified : Thursday, May 09, 2019 11:20:36 AM
Signals calculated separately : No

Rel. Reference Window : 0.000 %
Abs. Reference Window : 0.100 min
Rel. Non-ref. Window : 0.000 %
Abs. Non-ref. Window : 0.100 min
Uncalibrated Peaks : not reported
Partial Calibration : Yes, identified peaks are recalibrated
Correct All Ret. Times: No, only for identified peaks

Curve Type : Linear
Origin : Ignored
Weight : Equal

Recalibration Settings:
Average Response : Average all calibrations
Average Retention Time: Floating Average New 75%

Calibration Report Options :
Printout of recalibrations within a sequence:
 Calibration Table after Recalibration
 Normal Report after Recalibration
If the sequence is done with bracketing:
 Results of first cycle (ending previous bracket)

Default Sample ISTD Information (if not set in sample table):

ISTD #	ISTD Amount [g/100cc]	Name
1	1.00000	n-propanol
2	1.00000	n-propanol

Signal Details

Signal 1: FID1 A, Front Signal
Signal 2: FID2 B, Back Signal

Overview Table

JK

RT	Sig	Lvl	Amount [g/100cc]	Area	Rsp.Factor	Ref	ISTD #	Compound
2.586	1	1	1.00000	3.69669	2.70512e-1	No	No 1	methanol
2.809	1	1	1.00000	4.26100	2.34687e-1	No	No 2	Acetaldehyde
2.977	2	1	1.00000	4.26100	2.34687e-1	No	No 2	Acetaldehyde
3.075	1	1	5.00000e-2	4.41218	1.13323e-2	No	No 1	ethanol
		2	1.00000e-1	8.93847	1.11876e-2			
		3	2.00000e-1	18.03616	1.10888e-2			
		4	3.00000e-1	26.76689	1.12079e-2			
		5	5.00000e-1	44.75016	1.11731e-2			
3.388	2	1	1.00000	4.26062	2.34707e-1	No	No 2	methanol
3.628	1	1	1.00000	9.73055	1.02769e-1	No	No 1	isopropyl alcohol
4.285	2	1	5.00000e-2	4.58750	1.08992e-2	No	No 2	ethanol
		2	1.00000e-1	9.24911	1.08119e-2			
		3	2.00000e-1	18.85801	1.06056e-2			
		4	3.00000e-1	28.08107	1.06834e-2			
		5	5.00000e-1	47.43238	1.05413e-2			
4.308	1	1	1.00000	6.49940	1.53860e-1	No	No 1	acetone
4.620	1	1	1.00000	46.58786	2.14648e-2	No	Yes 1	n-propanol
		2	1.00000	47.95212	2.08541e-2			
		3	1.00000	48.16090	2.07637e-2			
		4	1.00000	47.10820	2.12277e-2			
		5	1.00000	47.54111	2.10344e-2			
4.661	2	1	1.00000	6.89301	1.45075e-1	No	No 2	acetone
4.969	2	1	1.00000	10.70642	9.34019e-2	No	No 2	isopropyl alcohol
7.550	2	1	1.00000	48.71809	2.05263e-2	No	Yes 2	n-propanol
		2	1.00000	49.83683	2.00655e-2			
		3	1.00000	49.84030	2.00641e-2			
		4	1.00000	48.64799	2.05558e-2			
		5	1.00000	48.97371	2.04191e-2			


Peak Sum Table

No Entries in table

1 Warnings or Errors :


Warning : Curve requires more calibration points., (methanol)

Calibration Curves

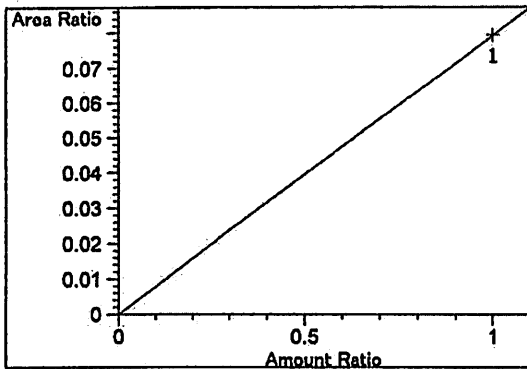


methanol at exp. RT: 2.586
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 7.93489e-2
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio


36

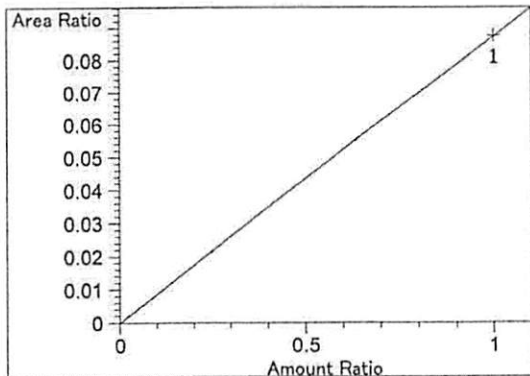


Acetaldehyde at exp. RT: 2.809
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 8.74624e-2
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio

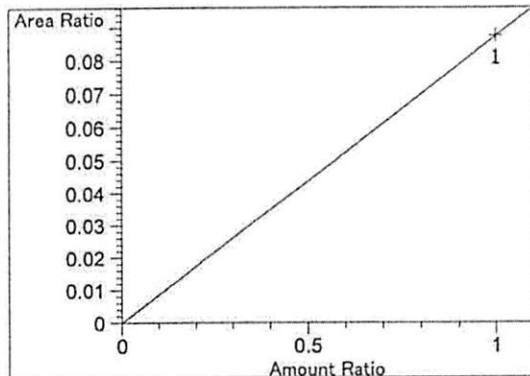

Acetaldehyde at exp. RT: 2.977
 FID2 B, Back Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 8.74624e-2
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio

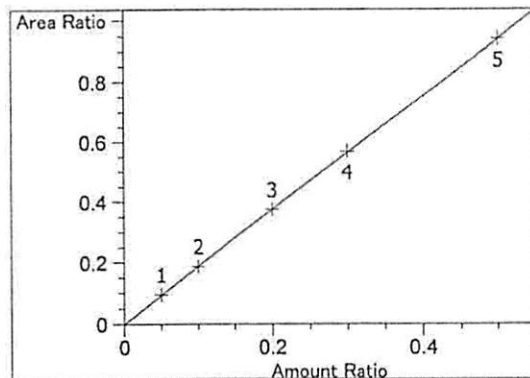


ethanol at exp. RT: 3.075
 FID1 A, Front Signal
 Correlation: 0.99998
 Residual Std. Dev.: 0.00245
 Formula: $y = mx + b$
 m: 1.88601
 b: -7.60614e-4
 x: Amount Ratio
 y: Area Ratio

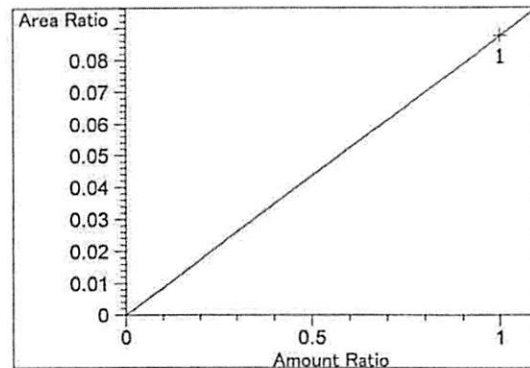


methanol at exp. RT: 3.388
 FID2 B, Back Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 8.74547e-2
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio


JK

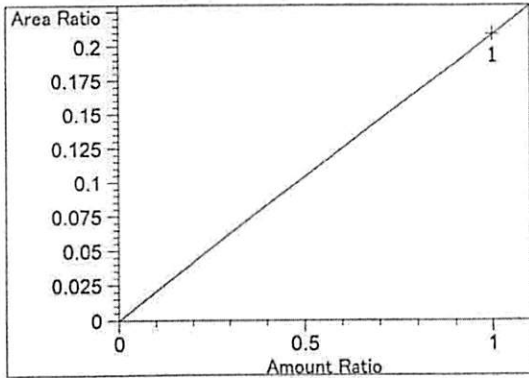


isopropyl alcohol at exp. RT: 3.628
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 2.08865e-1
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio

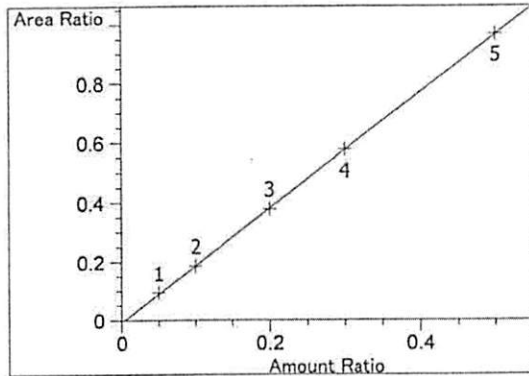

ethanol at exp. RT: 4.285
 FID2 B, Back Signal
 Correlation: 0.99996
 Residual Std. Dev.: 0.00360
 Formula: $y = mx + b$
 m: 1.94907
 b: -7.51137e-3
 x: Amount Ratio
 y: Area Ratio

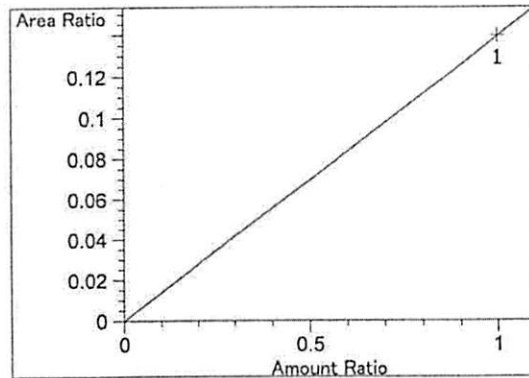


acetone at exp. RT: 4.308
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 1.39508e-1
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio

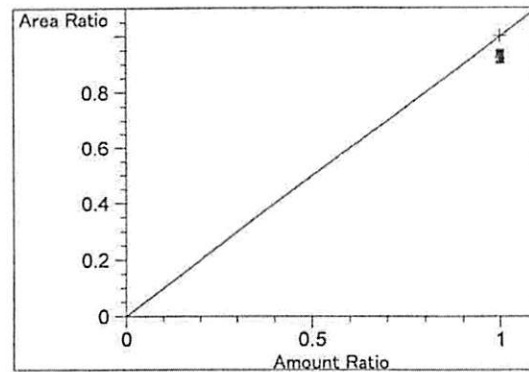


n-propanol at exp. RT: 4.620
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 1.00000
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio


dk

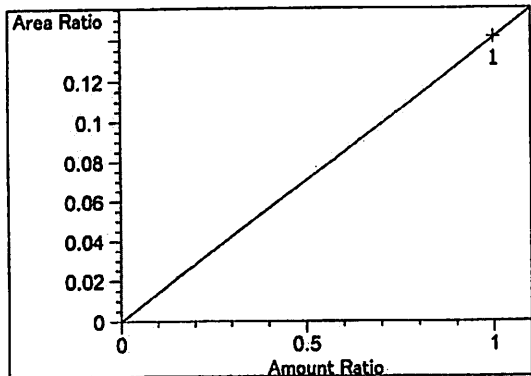

acetone at exp. RT: 4.661
FID2 B, Back Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx + b$
m: 1.41488e-1
b: 0.00000
x: Amount Ratio
y: Area Ratio

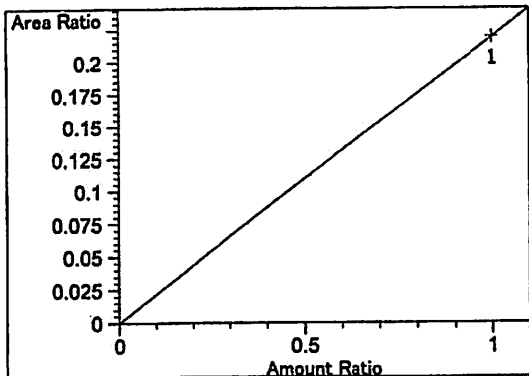

isopropyl alcohol at exp. RT: 4.969
FID2 B, Back Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx + b$
m: 2.19763e-1
b: 0.00000
x: Amount Ratio
y: Area Ratio

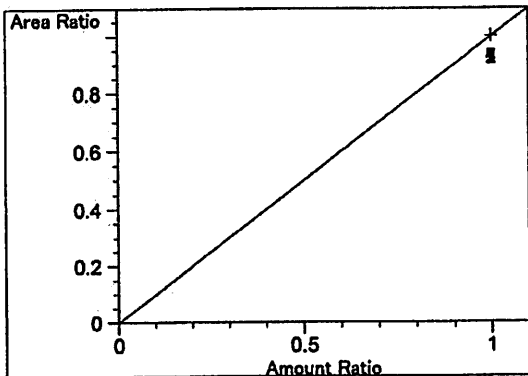


n-propanol at exp. RT: 7.550
FID2 B, Back Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx + b$
m: 1.00000
b: 0.00000
x: Amount Ratio
y: Area Ratio

dg

ISP Forensic Services Blood Alcohol Report


Sample Name : INTERNAL STD BLK 1
 Laboratory : Meridian
 Injection Date : May 16, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

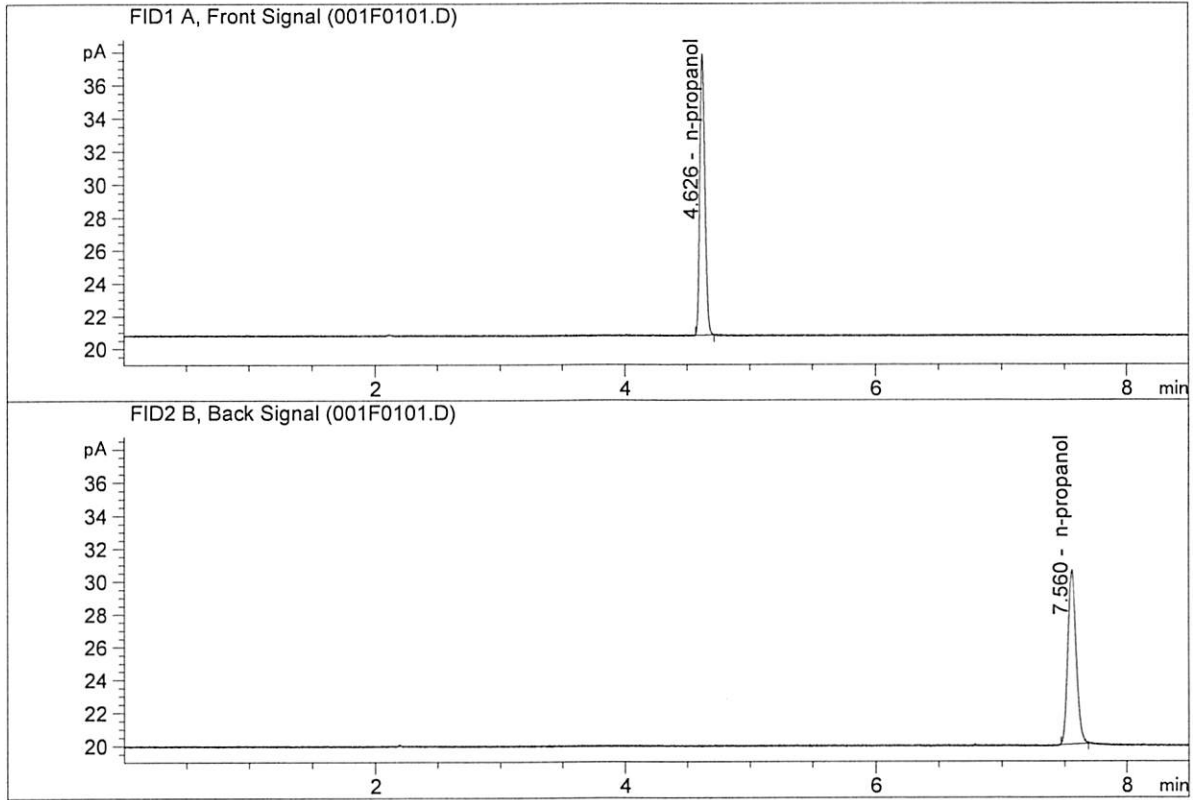

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	48.52590	1.0000	g/100cc
4.	n-Propanol	Column 2:	50.73167	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report

Sample Name : MIX VOL FN06041502
 Laboratory : Meridian
 Injection Date : May 16, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

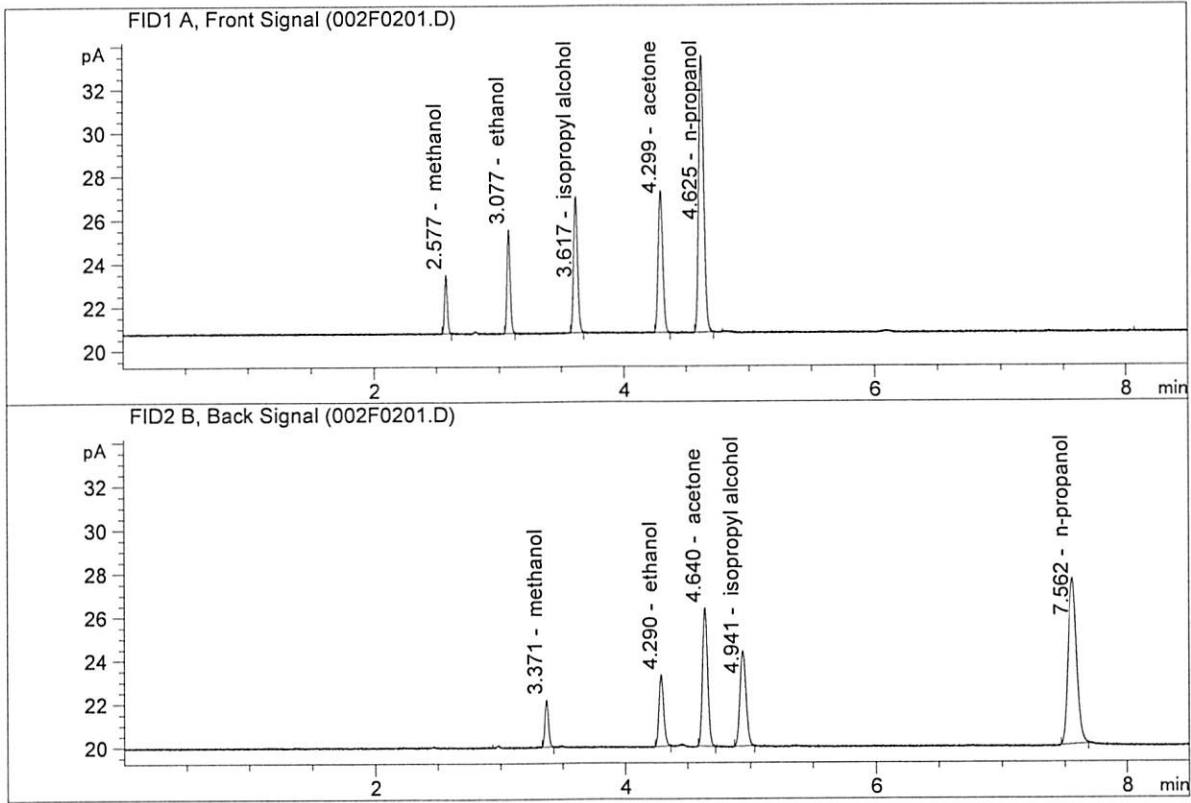

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	8.42277	0.1251	g/100cc
2.	Ethanol	Column 2:	8.69686	0.1256	g/100cc
3.	n-Propanol	Column 1:	35.81040	1.0000	g/100cc
4.	n-Propanol	Column 2:	36.65882	1.0000	g/100cc

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC1-1

Analysis Date(s): 16 May 2019

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean
Sample Results	0.0798	0.0803	0.0005	0.0800	0.0799
(g/100cc)	0.0799	0.0798	0.0001	0.0798	

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: Alcohol.m
Hamilton Auto-Dilutor Serial Number: ML600HC11378

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.079	0.075	0.083	0.004


Reported Result	
0.079	

Calibration and control data are stored centrally.

36

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-1-A
 Laboratory : Meridian
 Injection Date : May 16, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

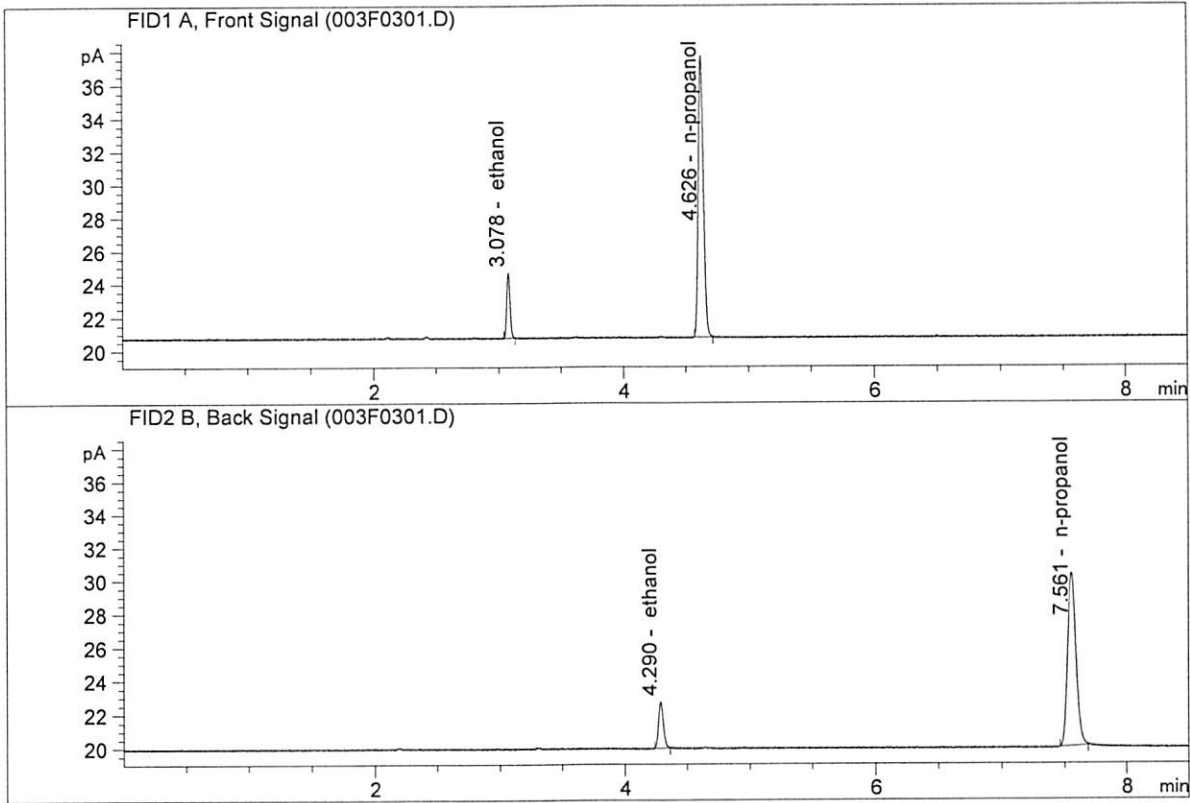


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.20005	0.0798	g/100cc
2.	Ethanol	Column 2:	7.39708	0.0803	g/100cc
3.	n-Propanol	Column 1:	48.08379	1.0000	g/100cc
4.	n-Propanol	Column 2:	49.65989	1.0000	g/100cc

JG

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-1-B
 Laboratory : Meridian
 Injection Date : May 16, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

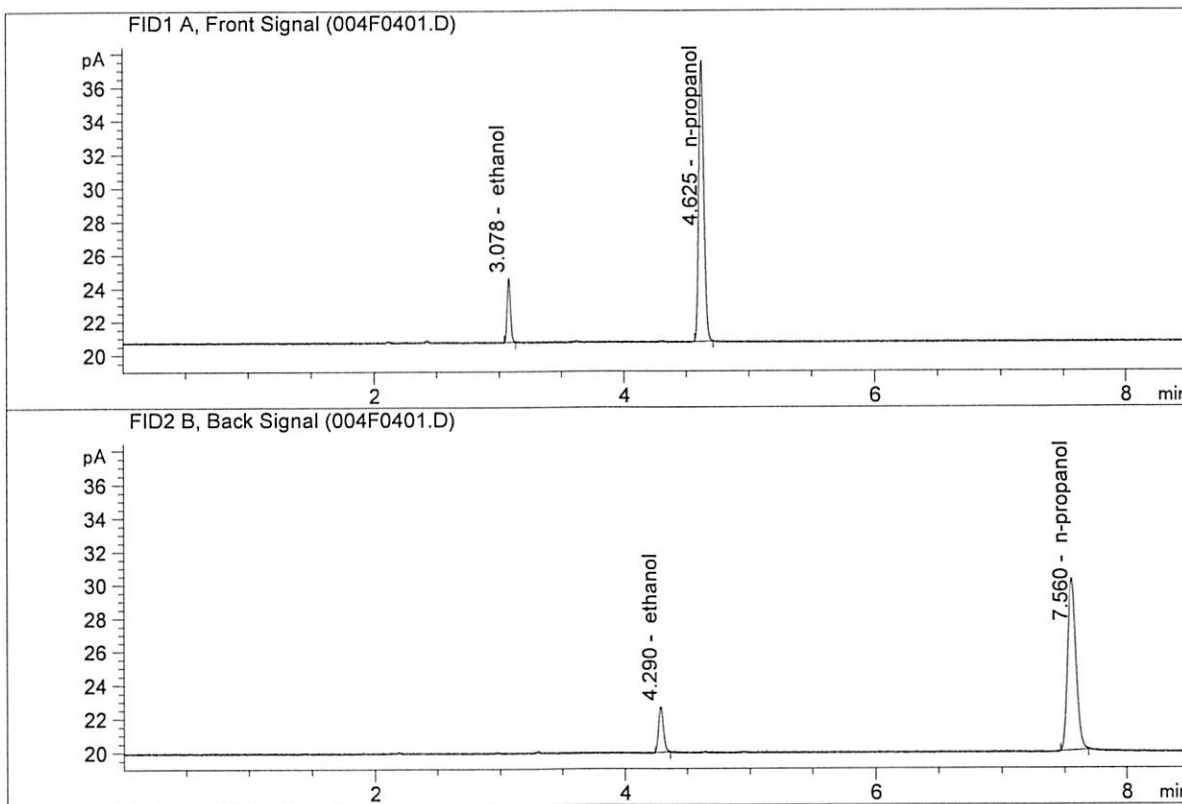

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.15367	0.0799	g/100cc
2.	Ethanol	Column 2:	7.30035	0.0798	g/100cc
3.	n-Propanol	Column 1:	47.72313	1.0000	g/100cc
4.	n-Propanol	Column 2:	49.32713	1.0000	g/100cc

JK

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: 0.08 FN04171701

Analysis Date(s): 16 May 2019

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.0805	0.0804	0.0001	0.0804	0.0804	
(g/100cc)	0.0800	0.0807	0.0007	0.0803		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: Alcohol.m
Hamilton Auto-Dilutor Serial Number: ML600HC11378

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.080	0.076	0.084	0.004

	Reported Result	
	0.080	

Calibration and control data are stored centrally.


Revision: 1

Issue Date: 01/04/2019

Issuing Authority: Quality Manager

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.08 FN04171701-A
 Laboratory : Meridian
 Injection Date : May 16, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

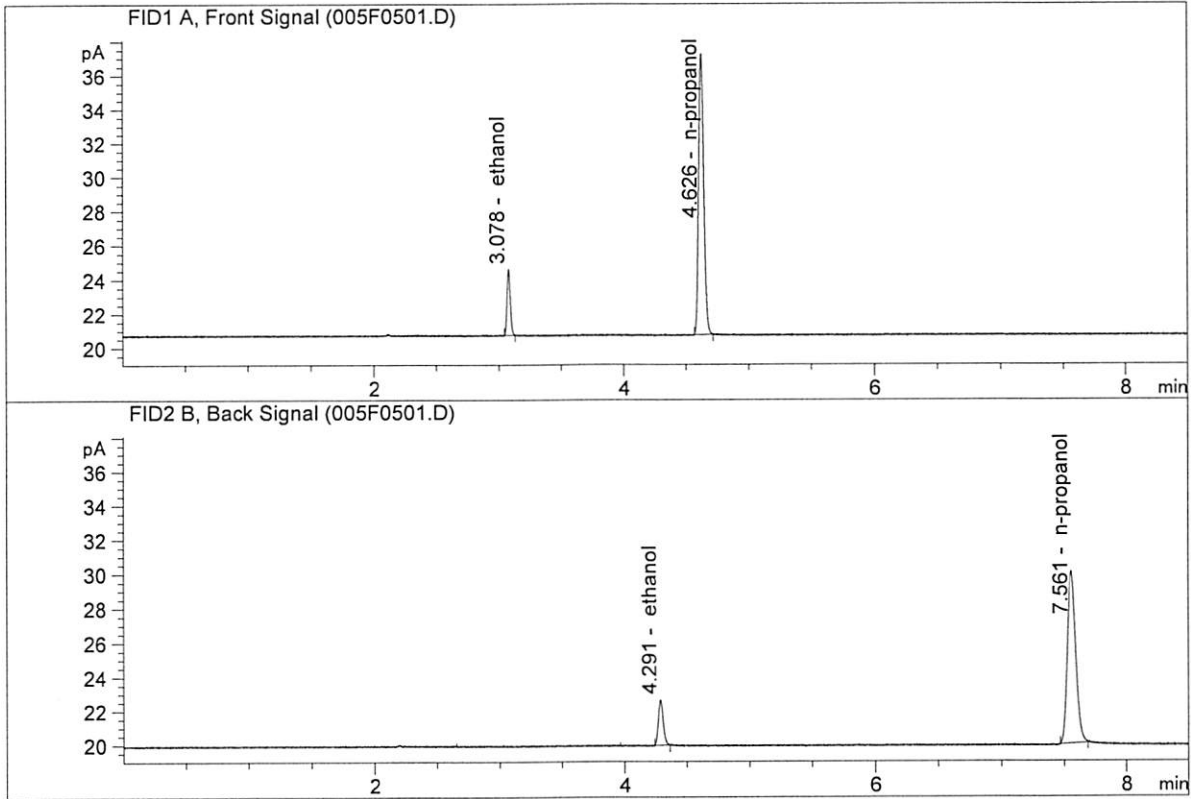


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.08330	0.0805	g/100cc
2.	Ethanol	Column 2:	7.21425	0.0804	g/100cc
3.	n-Propanol	Column 1:	46.90722	1.0000	g/100cc
4.	n-Propanol	Column 2:	48.37540	1.0000	g/100cc

JG

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.08 FN04171701-B
 Laboratory : Meridian
 Injection Date : May 16, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

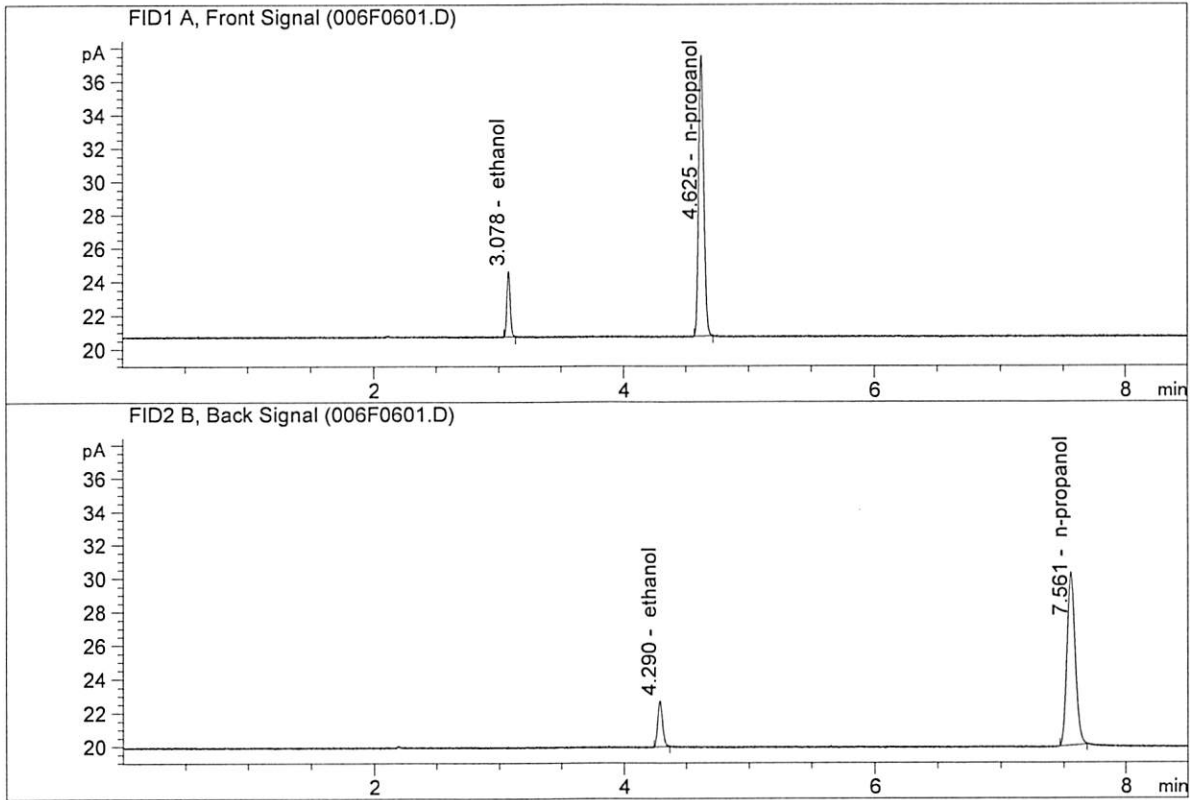

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.17281	0.0800	g/100cc
2.	Ethanol	Column 2:	7.36766	0.0807	g/100cc
3.	n-Propanol	Column 1:	47.76482	1.0000	g/100cc
4.	n-Propanol	Column 2:	49.17622	1.0000	g/100cc

JC

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC2-1

Analysis Date(s): 16 May 2019

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.2037	0.2041	0.0004	0.2039	0.2042	
(g/100cc)	0.2048	0.2044	0.0004	0.2046		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: Alcohol.m
Hamilton Auto-Dilutor Serial Number: ML600HC11378

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.204	0.193	0.215	0.011


	Reported Result	
	0.204	

Calibration and control data are stored centrally.

JG

ISP Forensic Services Blood Alcohol Report


Sample Name : QC2-1-A
 Laboratory : Meridian
 Injection Date : May 16, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

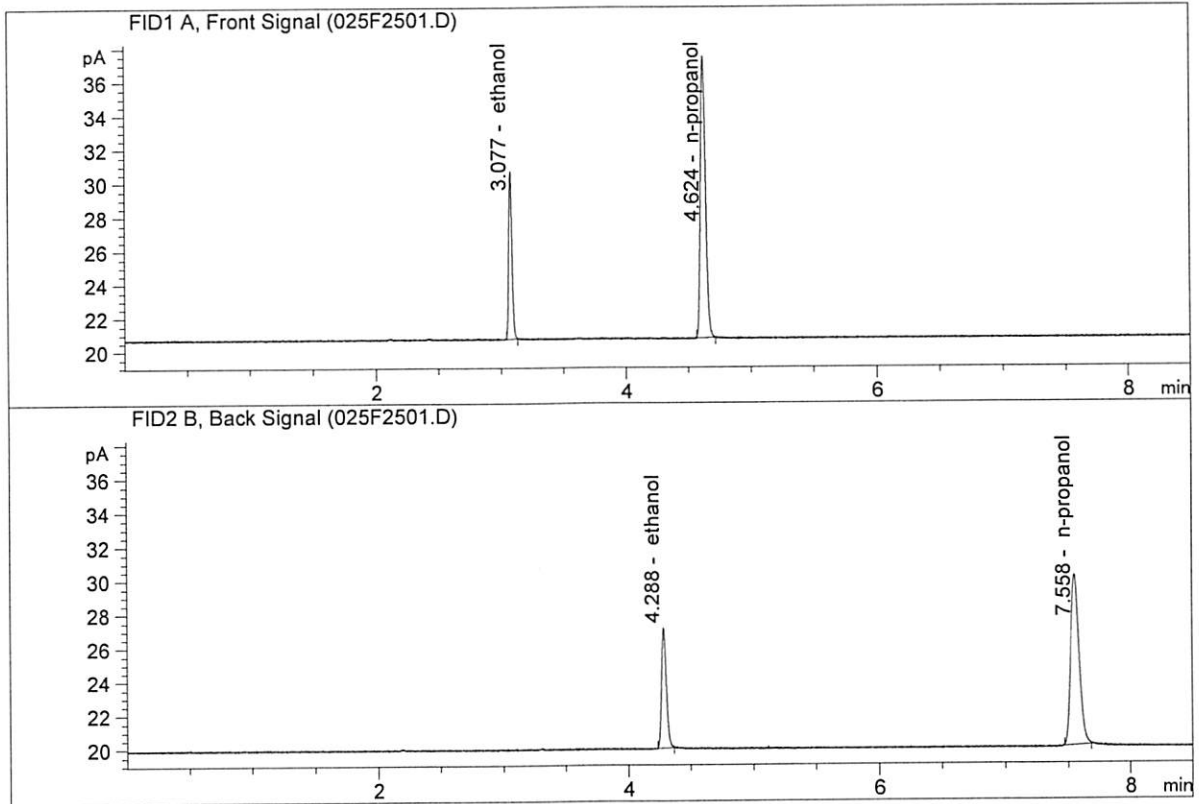

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	18.16175	0.2037	g/100cc
2.	Ethanol	Column 2:	18.93568	0.2041	g/100cc
3.	n-Propanol	Column 1:	47.35787	1.0000	g/100cc
4.	n-Propanol	Column 2:	48.52747	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report

Sample Name : QC2-1-B
 Laboratory : Meridian
 Injection Date : May 16, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

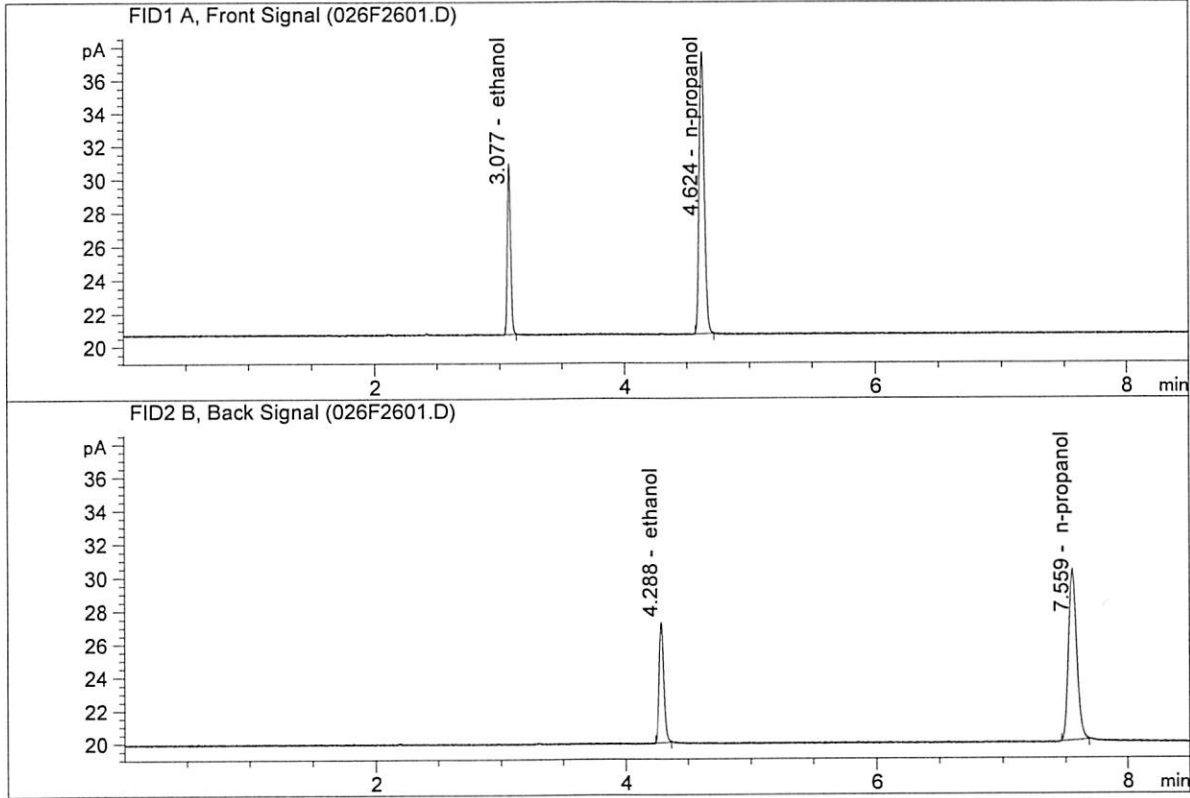

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	18.60356	0.2048	g/100cc
2.	Ethanol	Column 2:	19.36563	0.2044	g/100cc
3.	n-Propanol	Column 1:	48.26687	1.0000	g/100cc
4.	n-Propanol	Column 2:	49.54420	1.0000	g/100cc

JG

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC1-2

Analysis Date(s): 16 May 2019

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.0844	0.0852	0.0008	0.0848	0.0851	
(g/100cc)	0.0853	0.0856	0.0003	0.0854		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: Alcohol.m
Hamilton Auto-Dilutor Serial Number: ML600HC11378

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.085	0.080	0.090	0.005

	Reported Result	
	0.085	

Calibration and control data are stored centrally.

JG


Revision: 1

Issue Date: 01/04/2019

Issuing Authority: Quality Manager

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-2-A
 Laboratory : Meridian
 Injection Date : May 16, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

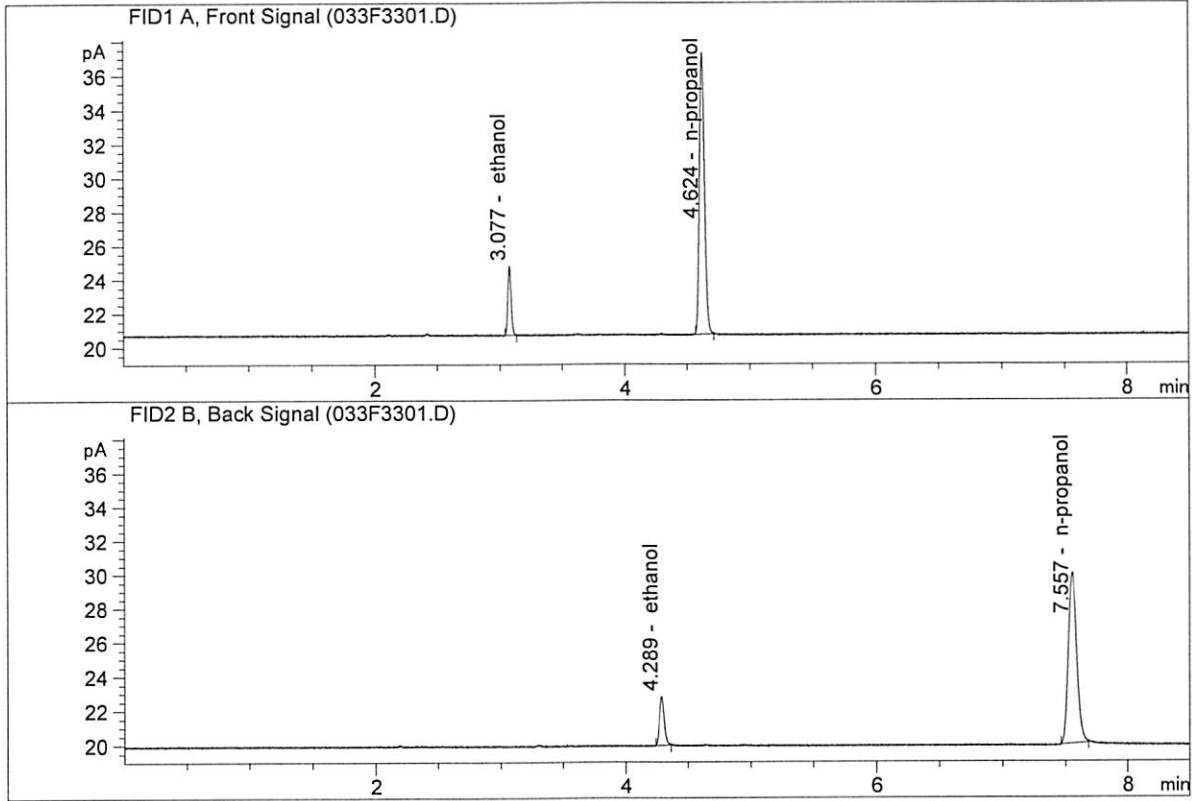


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.44372	0.0844	g/100cc
2.	Ethanol	Column 2:	7.62053	0.0852	g/100cc
3.	n-Propanol	Column 1:	46.97370	1.0000	g/100cc
4.	n-Propanol	Column 2:	48.08801	1.0000	g/100cc

JG

ISP Forensic Services Blood Alcohol Report


Sample Name : QC1-2-B
 Laboratory : Meridian
 Injection Date : May 16, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

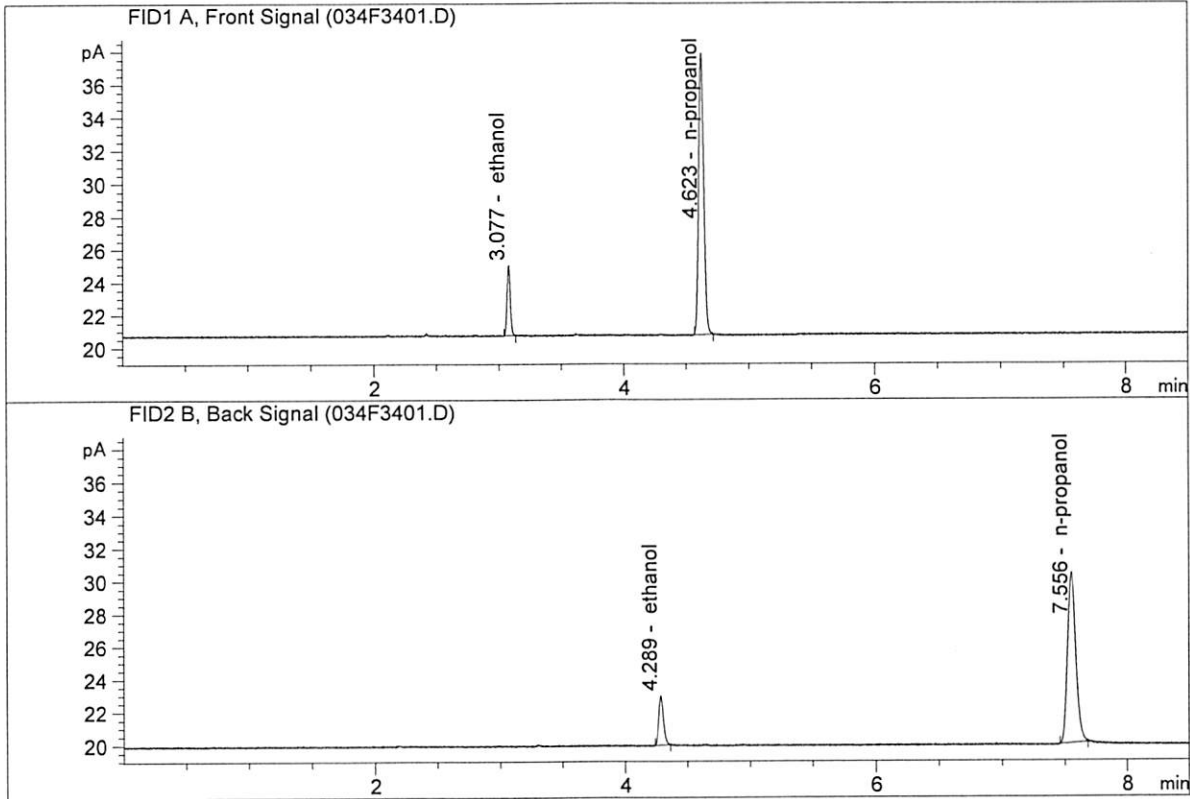

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.77466	0.0853	g/100cc
2.	Ethanol	Column 2:	7.92979	0.0856	g/100cc
3.	n-Propanol	Column 1:	48.58332	1.0000	g/100cc
4.	n-Propanol	Column 2:	49.76263	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report

Sample Name : BLK
 Laboratory : Meridian
 Injection Date : May 16, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

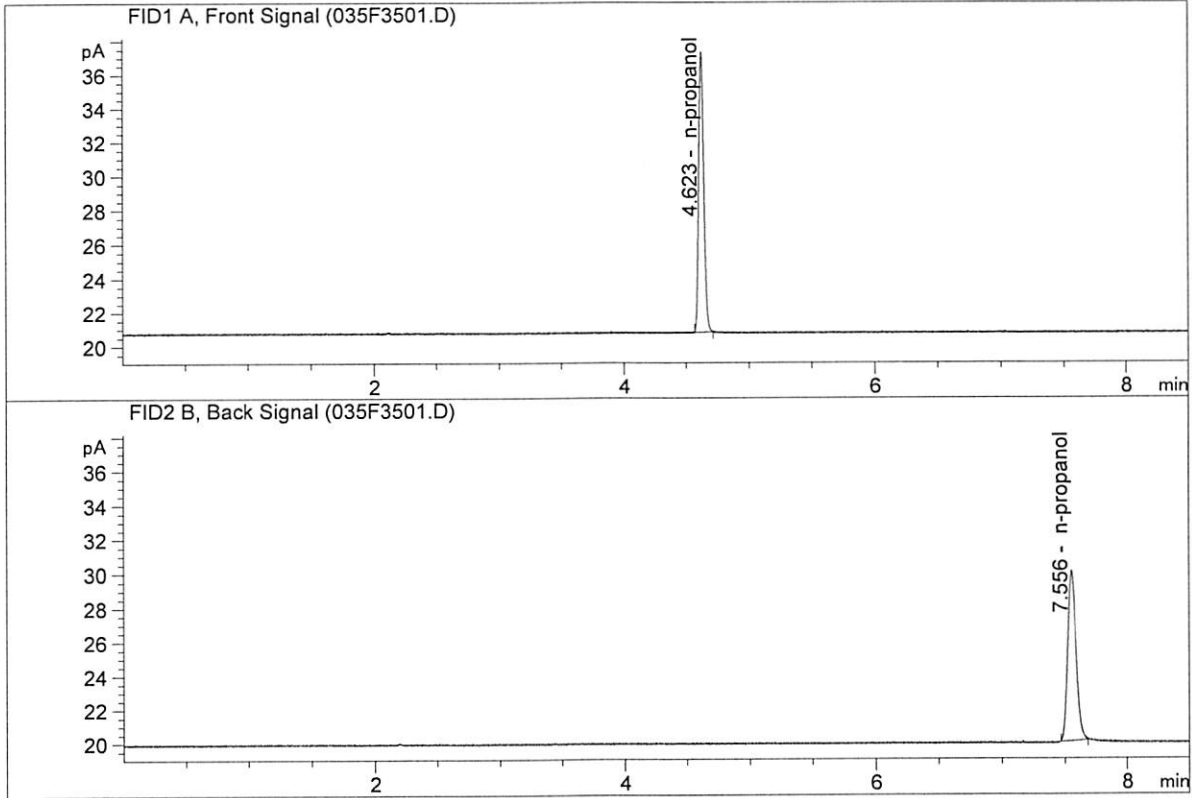

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	46.92456	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.98353	1.0000	g/100cc

S a m p l e S u m m a r y

Sequence table: C:\Chem32\1\Data\05-16-19_SAMPLES\05-16-19_SAMPLES 2019-05-16 14-45-58\05-16-19_SAMPLES.S
 Data directory path: C:\Chem32\1\Data\05-16-19_SAMPLES\05-16-19_SAMPLES 2019-05-16 14-45-58\
 Logbook: C:\Chem32\1\Data\05-16-19_SAMPLES\05-16-19_SAMPLES 2019-05-16 14-45-58\05-16-19_SAMPLES.LOG
 Sequence start: 5/16/2019 3:00:46 PM
 Sequence Operator: SYSTEM
 Operator: SYSTEM
 Method file name: C:\Chem32\1\Data\05-16-19_SAMPLES\05-16-19_SAMPLES 2019-05-16 14-45-58\ALCOHOL.M

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal # Cmp
1	1	1	INTERNAL STD BLK	-	1.0000	001F0101.D	2
2	2	1	MIX VOL FN060415	-	1.0000	002F0201.D	10
3	3	1	QC1-1-A	-	1.0000	003F0301.D	4
4	4	1	QC1-1-B	-	1.0000	004F0401.D	4
5	5	1	0.08 FN04171701-	-	1.0000	005F0501.D	4
6	6	1	0.08 FN04171701-	-	1.0000	006F0601.D	4
7	7	1	M2019-2164-1-A	-	1.0000	007F0701.D	2
8	8	1	M2019-2164-1-B	-	1.0000	008F0801.D	2
9	9	1	M2019-2174-2-A	-	1.0000	009F0901.D	2
10	10	1	M2019-2174-2-B	-	1.0000	010F1001.D	2
11	11	1	M2019-2199-1-A	-	1.0000	011F1101.D	2
12	12	1	M2019-2199-1-B	-	1.0000	012F1201.D	2
13	13	1	M2019-2203-1-A	-	1.0000	013F1301.D	4
14	14	1	M2019-2203-1-B	-	1.0000	014F1401.D	4
15	15	1	M2019-2224-1-A	-	1.0000	015F1501.D	4
16	16	1	M2019-2224-1-B	-	1.0000	016F1601.D	4
17	17	1	M2019-2225-1-A	-	1.0000	017F1701.D	4
18	18	1	M2019-2225-1-B	-	1.0000	018F1801.D	4
19	19	1	M2019-2226-1-A	-	1.0000	019F1901.D	4
20	20	1	M2019-2226-1-B	-	1.0000	020F2001.D	4
21	21	1	M2019-2227-1-A	-	1.0000	021F2101.D	4
22	22	1	M2019-2227-1-B	-	1.0000	022F2201.D	4
23	23	1	M2019-2244-1-A	-	1.0000	023F2301.D	4
24	24	1	M2019-2244-1-B	-	1.0000	024F2401.D	4
25	25	1	QC2-1-A	-	1.0000	025F2501.D	4
26	26	1	QC2-1-B	-	1.0000	026F2601.D	4
27	27	1	M2019-2261-1-A	-	1.0000	027F2701.D	4
28	28	1	M2019-2261-1-B	-	1.0000	028F2801.D	4
29	29	1	M2019-2262-1-A	-	1.0000	029F2901.D	2
30	30	1	M2019-2262-1-B	-	1.0000	030F3001.D	2
31	31	1	M2019-2278-1-A	-	1.0000	031F3101.D	4
32	32	1	M2019-2278-1-B	-	1.0000	032F3201.D	4
33	33	1	QC1-2-A	-	1.0000	033F3301.D	4
34	34	1	QC1-2-B	-	1.0000	034F3401.D	4
35	35	1	BLK	-	1.0000	035F3501.D	2

06

Method file name: C:\Chem32\1\Data\05-16-19_SAMPLES\05-16-19_SAMPLES 2019-05-16 14-45-58
\SHUTDOWN.M

Run #	Location	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #
36	36	1	SHUTDOWN	-	1.0000	036F3601.D	0

06