

Quantitative Analysis for Ethanol & Qualitative Analysis for Other Volatiles

Analytical Method(s): 1.0

Device: Hamilton MICROLAB 600A Liquid Processor/Dilutor Serial Number: ML600HC11378

Volatiles Quality Assurance Controls Run Date(s):7/2/19-7/3/19

Calibration Date: 7/2/19

Control level	Expiration	Lot #	Target Value	Acceptable Range	Overall Results
Level 1	Jan-22	1801036	0.0812	0.0731-0.0893	0.0803 g/100cc
					0.0842 g/100cc
Level 2	Mar-22	1803028	0.2035	0.1832-0.2238	0.2046 g/100cc
					g/100cc
Multi-Component mixture:		Sep-20	Lot #	FN06041502	ok
Curve Fit:		Column 1	1.00000	Column2	0.99992

Ethanol Calibration Reference Material						
Calibrator level	Target Value	Acceptable Range	Column 1	Column 2	Precision	Mean
50	0.050	0.045 - 0.055	0.0505	0.0524	0.0019	0.0514
100	0.100	0.090 - 0.110	0.1000	0.1002	0.0002	0.1001
200	0.200	0.180 - 0.220	0.1992	0.1972	0.002	0.1982
300	0.300	0.270 - 0.330	0.3000	0.2983	0.0017	0.2991
500	0.500	0.450 - 0.550	0.5003	0.5019	0.0016	0.5011

Aqueous Controls			
Control level	Target Value	Acceptable Range	Overall Results
80	0.080	0.076 - 0.084	0.080 g/100cc

REVIEWED















By Jeremy Johnson at 1:37 pm, Jul 05, 2019

✓

Revision: 1

Issue Date: 01/03/2019

Worklist: 3524

<u>LAB CASE</u>	<u>ITEM</u>	<u>TASK ID</u>	<u>DESCRIPTION</u>	
M2019-2773	1	155248	Alcohol Analysis	
M2019-2774	1	155255	Alcohol Analysis	
M2019-2775	1	155256	Alcohol Analysis	
M2019-2776	1	155257	Alcohol Analysis	
M2019-2783	1	155305	Alcohol Analysis	
M2019-2859	1	155563	Alcohol Analysis	
M2019-2860	1	155564	Alcohol Analysis	
M2019-2870	1	155608	Alcohol Analysis	
M2019-2882	1	155633	Alcohol Analysis	
M2019-2908	1	155880	Alcohol Analysis	
M2019-2909	1	155882	Alcohol Analysis	
M2019-2944	1	156031	Alcohol Analysis	
M2019-2981	1	156194	Alcohol Analysis	
M2019-2998	1	156267	Alcohol Analysis	
M2019-2999	1	156271	Alcohol Analysis	
M2019-3000	1	156272	Alcohol Analysis	
M2019-3001	1	156276	Alcohol Analysis	
M2019-3002	1	156280	Alcohol Analysis	
M2019-3002	2	156281	Alcohol Analysis	

JG

=====
Calibration Table
=====

General Calibration Setting

Calib. Data Modified : Tuesday, July 02, 2019 4:08:55 PM
Signals calculated separately : No

Rel. Reference Window : 0.000 %
Abs. Reference Window : 0.100 min
Rel. Non-ref. Window : 0.000 %
Abs. Non-ref. Window : 0.100 min
Uncalibrated Peaks : not reported
Partial Calibration : Yes, identified peaks are recalibrated
Correct All Ret. Times: No, only for identified peaks

Curve Type : Linear
Origin : Ignored
Weight : Equal

Recalibration Settings:
Average Response : Average all calibrations
Average Retention Time: Floating Average New 75%

Calibration Report Options :
Printout of recalibrations within a sequence:
 Calibration Table after Recalibration
 Normal Report after Recalibration
If the sequence is done with bracketing:
 Results of first cycle (ending previous bracket)

Default Sample ISTD Information (if not set in sample table):

ISTD #	ISTD Amount [g/100cc]	Name
1	1.00000	n-propanol
2	1.00000	n-propanol

Signal Details

Signal 1: FID1 A, Front Signal
Signal 2: FID2 B, Back Signal

Overview Table

JG

RT	Sig	Lvl	Amount [g/100cc]	Area	Rsp.Factor	Ref	ISTD #	Compound
2.586	1	1	1.00000	3.69669	2.70512e-1	No	No 1	methanol
2.809	1	1	1.00000	4.26100	2.34687e-1	No	No 2	Acetaldehyde
2.977	2	1	1.00000	4.26100	2.34687e-1	No	No 2	Acetaldehyde
3.075	1	1	5.00000e-2	4.42648	1.12957e-2	No	No 1	ethanol
			1.00000e-1	8.88798	1.12512e-2			
			2.00000e-1	17.84929	1.12049e-2			
			3.00000e-1	26.60101	1.12778e-2			
			5.00000e-1	45.10629	1.10849e-2			
3.388	2	1	1.00000	4.26062	2.34707e-1	No	No 2	methanol
3.628	1	1	1.00000	9.73055	1.02769e-1	No	No 1	isopropyl alcohol
4.285	2	1	5.00000e-2	4.61899	1.08249e-2	No	No 2	ethanol
			1.00000e-1	9.21829	1.08480e-2			
			2.00000e-1	18.62832	1.07363e-2			
			3.00000e-1	27.95925	1.07299e-2			
			5.00000e-1	47.84081	1.04513e-2			
4.308	1	1	1.00000	6.49940	1.53860e-1	No	No 1	acetone
4.620	1	1	1.00000	45.96296	2.17566e-2	No	Yes 1	n-propanol
			1.00000	45.94650	2.17644e-2			
			1.00000	46.01707	2.17311e-2			
			1.00000	45.42292	2.20153e-2			
			1.00000	46.10006	2.16919e-2			
4.661	2	1	1.00000	6.89301	1.45075e-1	No	No 2	acetone
4.969	2	1	1.00000	10.70642	9.34019e-2	No	No 2	isopropyl alcohol
7.550	2	1	1.00000	48.17994	2.07555e-2	No	Yes 2	n-propanol
			1.00000	47.85523	2.08964e-2			
			1.00000	47.86760	2.08910e-2			
			1.00000	47.08141	2.12398e-2			
			1.00000	47.54148	2.10343e-2			


Peak Sum Table

No Entries in table

1 Warnings or Errors :


Warning : Curve requires more calibration points., (methanol)

Calibration Curves

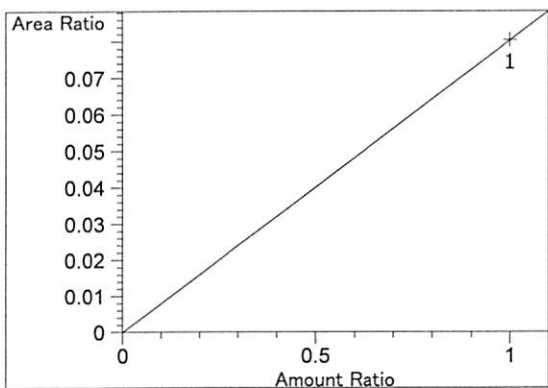


methanol at exp. RT: 2.586
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 8.04277e-2
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio


JK

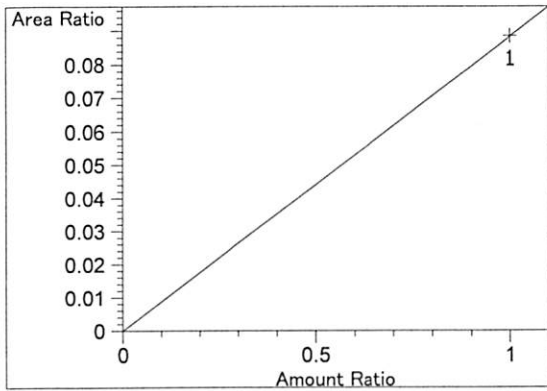


Acetaldehyde at exp. RT: 2.809
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 8.84393e-2
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio

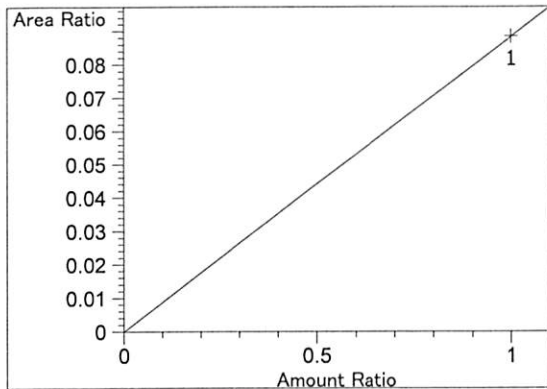

Acetaldehyde at exp. RT: 2.977
 FID2 B, Back Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 8.84393e-2
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio

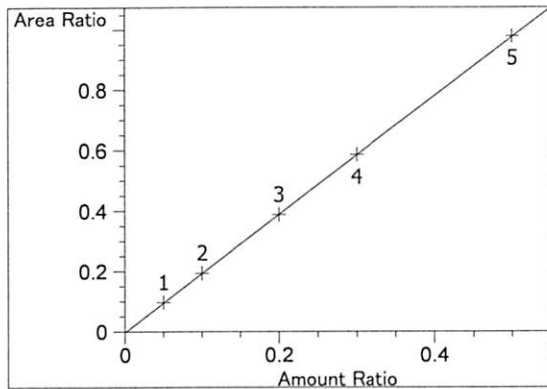


ethanol at exp. RT: 3.075
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00114
 Formula: $y = mx + b$
 m: 1.96137
 b: -2.77326e-3
 x: Amount Ratio
 y: Area Ratio

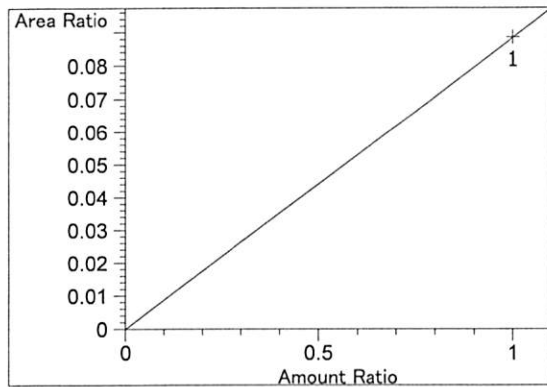


methanol at exp. RT: 3.388
 FID2 B, Back Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 8.84315e-2
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio


16

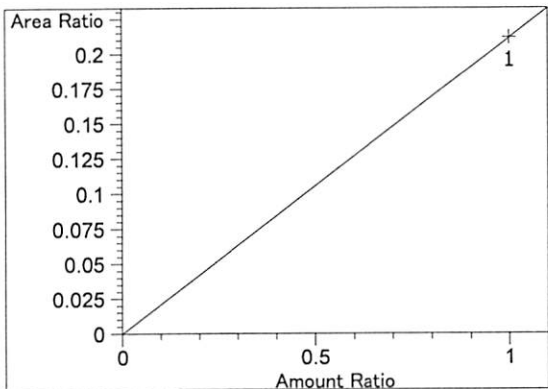


isopropyl alcohol at exp. RT: 3.628
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 2.11704e-1
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio

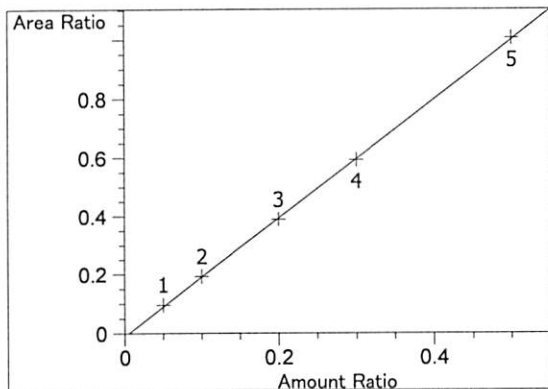

ethanol at exp. RT: 4.285
 FID2 B, Back Signal
 Correlation: 0.99992
 Residual Std. Dev.: 0.00526
 Formula: $y = mx + b$
 m: 2.02575
 b: -1.03615e-2
 x: Amount Ratio
 y: Area Ratio

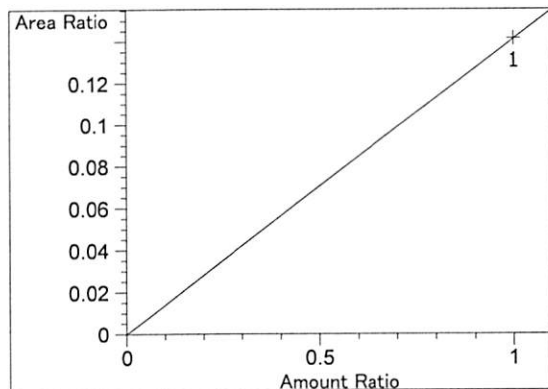


acetone at exp. RT: 4.308
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 1.41405e-1
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio

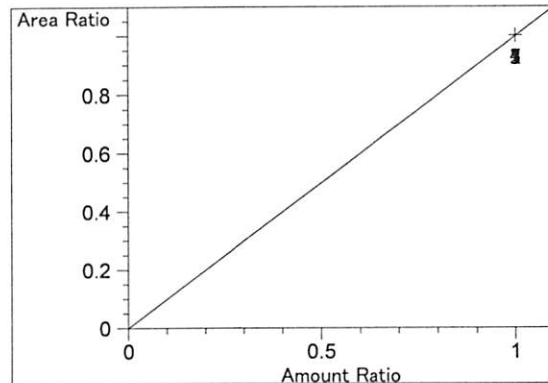


n-propanol at exp. RT: 4.620
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 1.00000
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio


JK

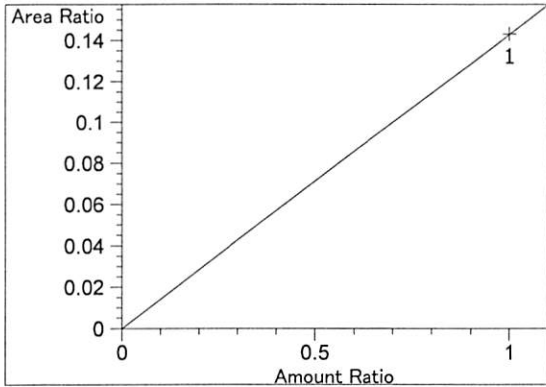

acetone at exp. RT: 4.661
FID2 B, Back Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx + b$
m: 1.43068e-1
b: 0.00000
x: Amount Ratio
y: Area Ratio

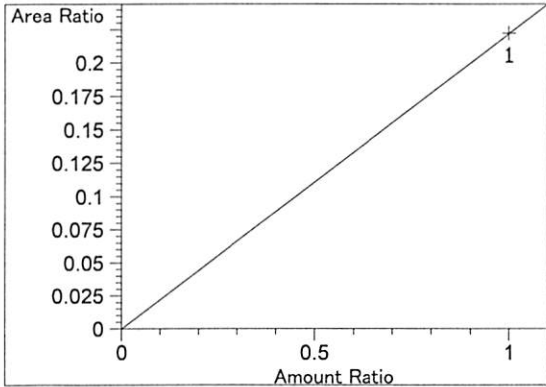

isopropyl alcohol at exp. RT: 4.969
FID2 B, Back Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx + b$
m: 2.22217e-1
b: 0.00000
x: Amount Ratio
y: Area Ratio

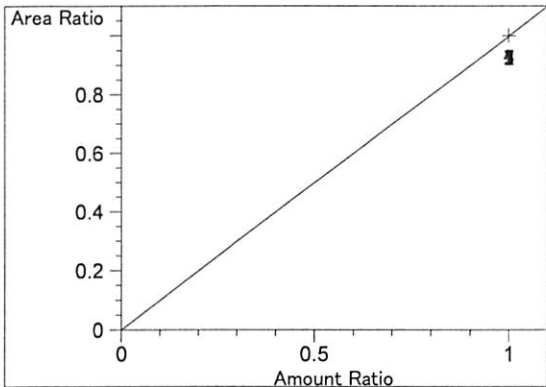


n-propanol at exp. RT: 7.550
FID2 B, Back Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx + b$
m: 1.00000
b: 0.00000
x: Amount Ratio
y: Area Ratio

=====

J6

ISP Forensic Services Blood Alcohol Report


Sample Name : 0.050 FN04271601
 Laboratory : Meridian
 Injection Date : Jul 2, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

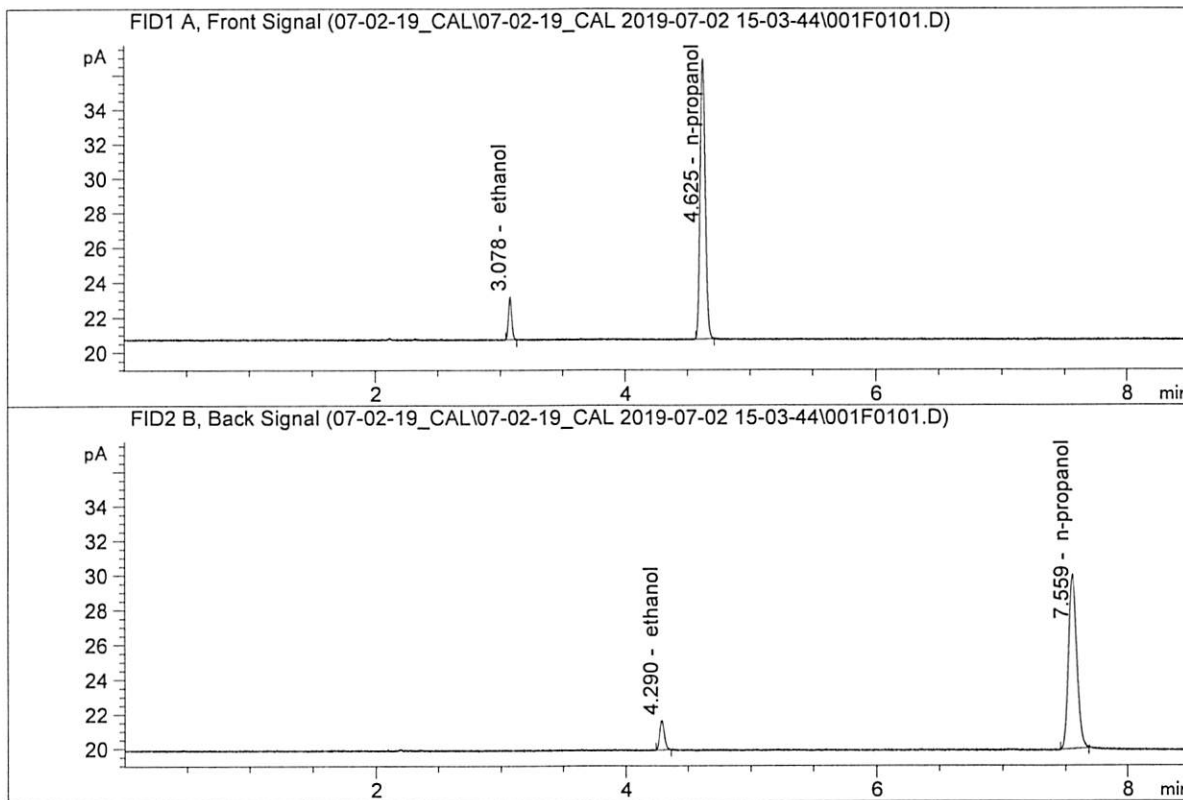

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	4.42648	0.0505	g/100cc
2.	Ethanol	Column 2:	4.61899	0.0524	g/100cc
3.	n-Propanol	Column 1:	45.96296	1.0000	g/100cc
4.	n-Propanol	Column 2:	48.17994	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.100 FN08101601
 Laboratory : Meridian
 Injection Date : Jul 2, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

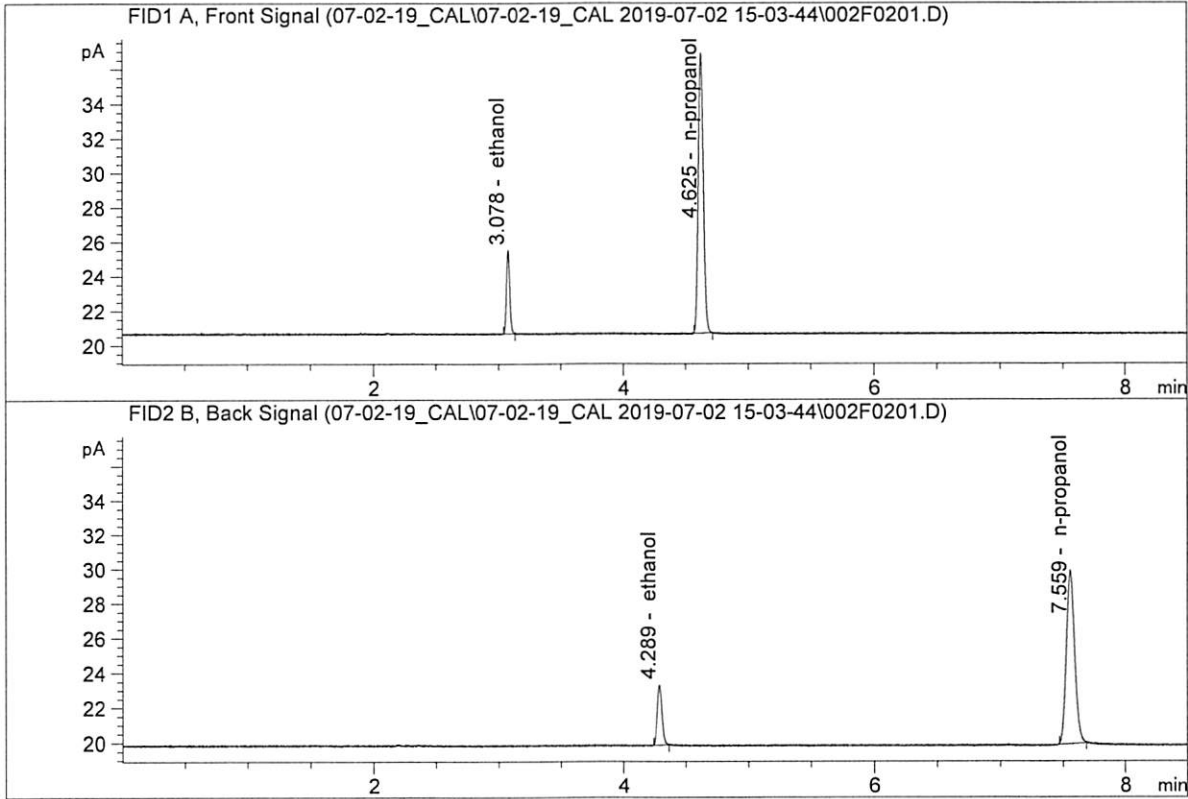


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	8.88798	0.1000	g/100cc
2.	Ethanol	Column 2:	9.21829	0.1002	g/100cc
3.	n-Propanol	Column 1:	45.94650	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.85523	1.0000	g/100cc

JG

ISP Forensic Services Blood Alcohol Report


Sample Name : 0.200 FN03301601
 Laboratory : Meridian
 Injection Date : Jul 2, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

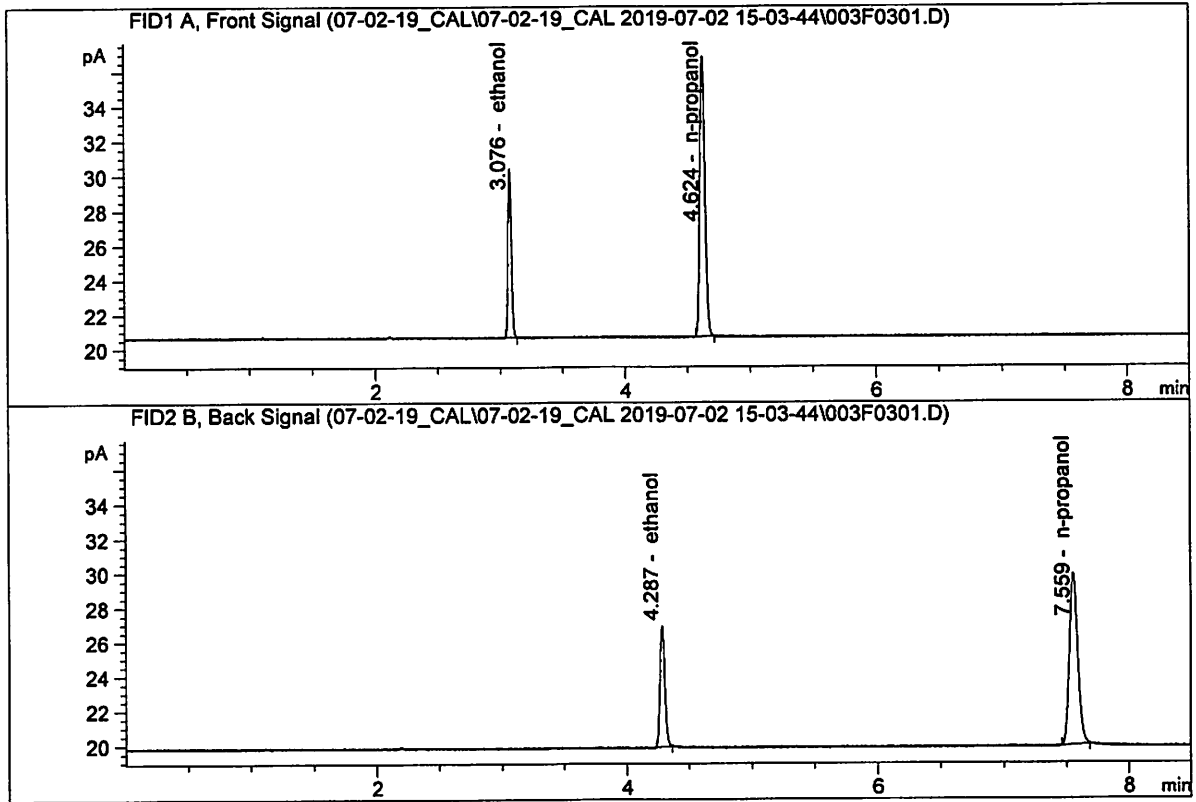

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	17.84929	0.1992	g/100cc
2.	Ethanol	Column 2:	18.62832	0.1972	g/100cc
3.	n-Propanol	Column 1:	46.01707	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.86760	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.300 FN02121601
 Laboratory : Meridian
 Injection Date : Jul 2, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

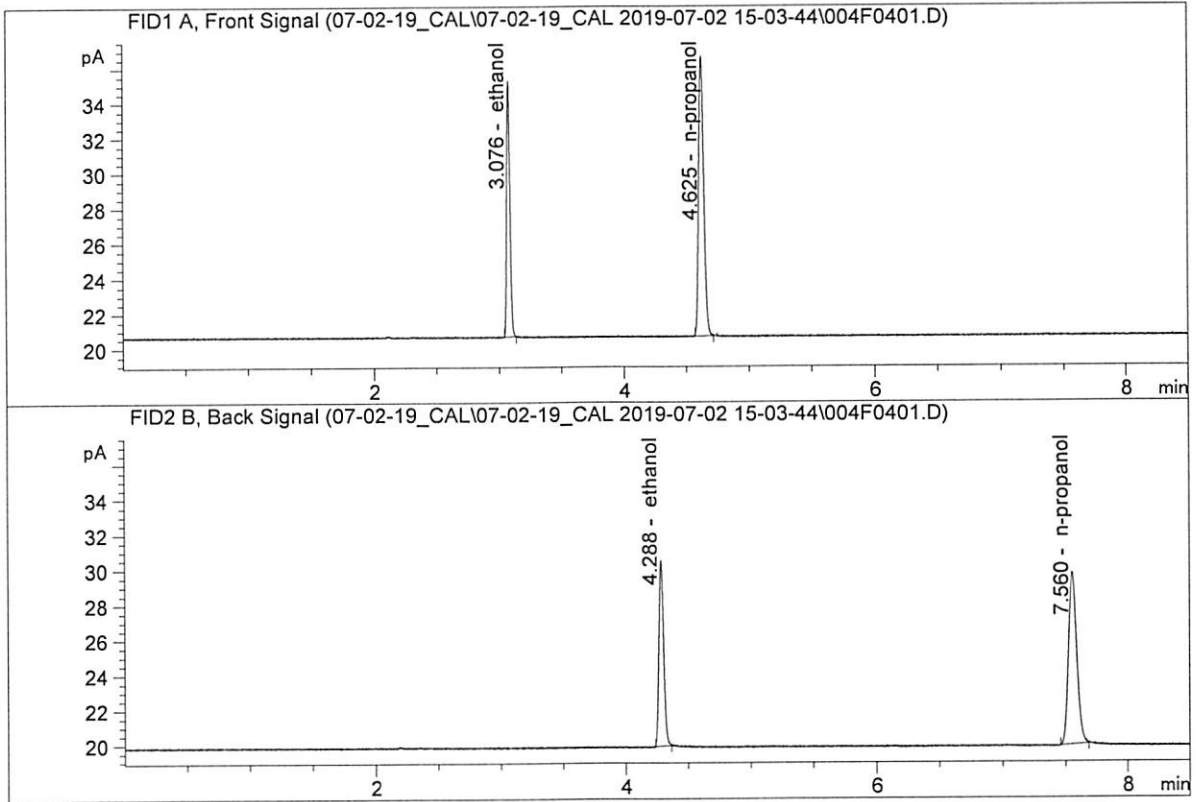


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	26.60101	0.3000	g/100cc
2.	Ethanol	Column 2:	27.95925	0.2983	g/100cc
3.	n-Propanol	Column 1:	45.42292	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.08141	1.0000	g/100cc

JK

ISP Forensic Services Blood Alcohol Report


Sample Name : 0.500 FN08031602
 Laboratory : Meridian
 Injection Date : Jul 2, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

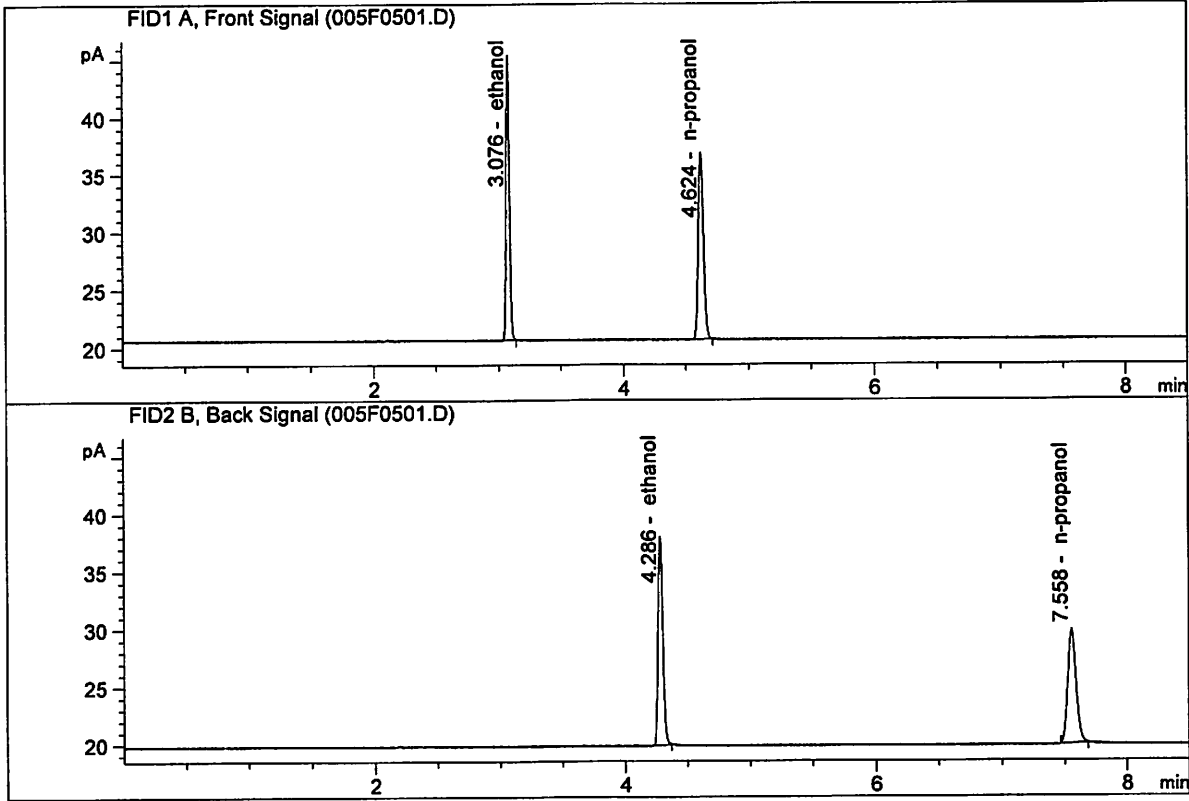

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	45.10629	0.5003	g/100cc
2.	Ethanol	Column 2:	47.84081	0.5019	g/100cc
3.	n-Propanol	Column 1:	46.10006	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.54148	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STANDARD BLANK
 Laboratory : Meridian
 Injection Date : Jul 2, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

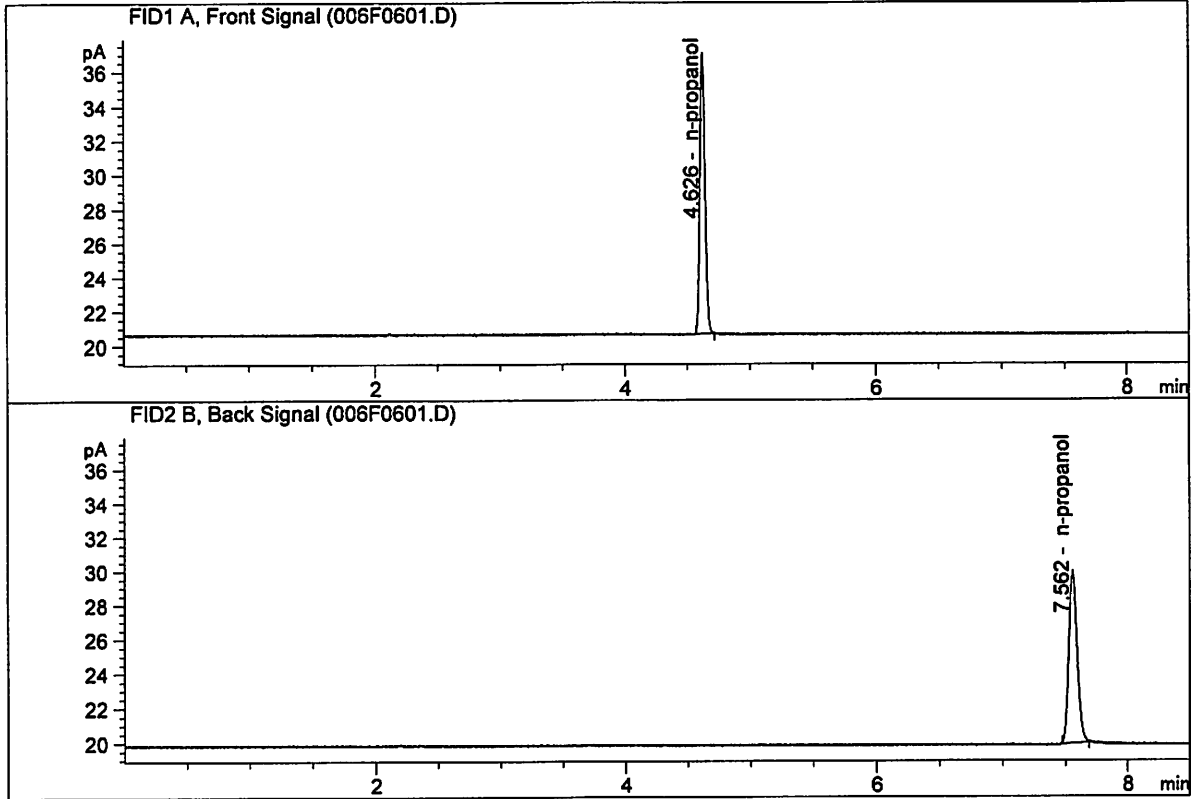

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	46.61699	1.0000	g/100cc
4.	n-Propanol	Column 2:	48.25599	1.0000	g/100cc

S a m p l e S u m m a r y

Sequence table: C:\Chem32\1\Data\07-02-19_CAL\07-02-19_CAL 2019-07-02 15-03-44\07-02-19_CAL.S
 Data directory path: C:\Chem32\1\Data\07-02-19_CAL\07-02-19_CAL 2019-07-02 15-03-44\
 Logbook: C:\Chem32\1\Data\07-02-19_CAL\07-02-19_CAL 2019-07-02 15-03-44\07-02-19_CAL.LOG
 Sequence start: 7/2/2019 3:18:24 PM
 Sequence Operator: SYSTEM
 Operator: SYSTEM


Method file name: C:\Chem32\1\Data\07-02-19_CAL\07-02-19_CAL 2019-07-02 15-03-44\ALCOHOL.M

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #	# Cmp
1	1	1	0.050 FN04271601	-	1.0000	001F0101.D	*	4
2	2	1	0.100 FN08101601	-	1.0000	002F0201.D	*	4
3	3	1	0.200 FN03301601	-	1.0000	003F0301.D	*	4
4	4	1	0.300 FN02121601	-	1.0000	004F0401.D	*	4
5	5	1	0.500 FN08031602	-	1.0000	005F0501.D	*	4
6	6	1	INTERNAL STANDAR	-	1.0000	006F0601.D		2

JG

ISP Forensic Services Blood Alcohol Report


Sample Name : INTERNAL STD BLK 1
 Laboratory : Meridian
 Injection Date : Jul 2, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

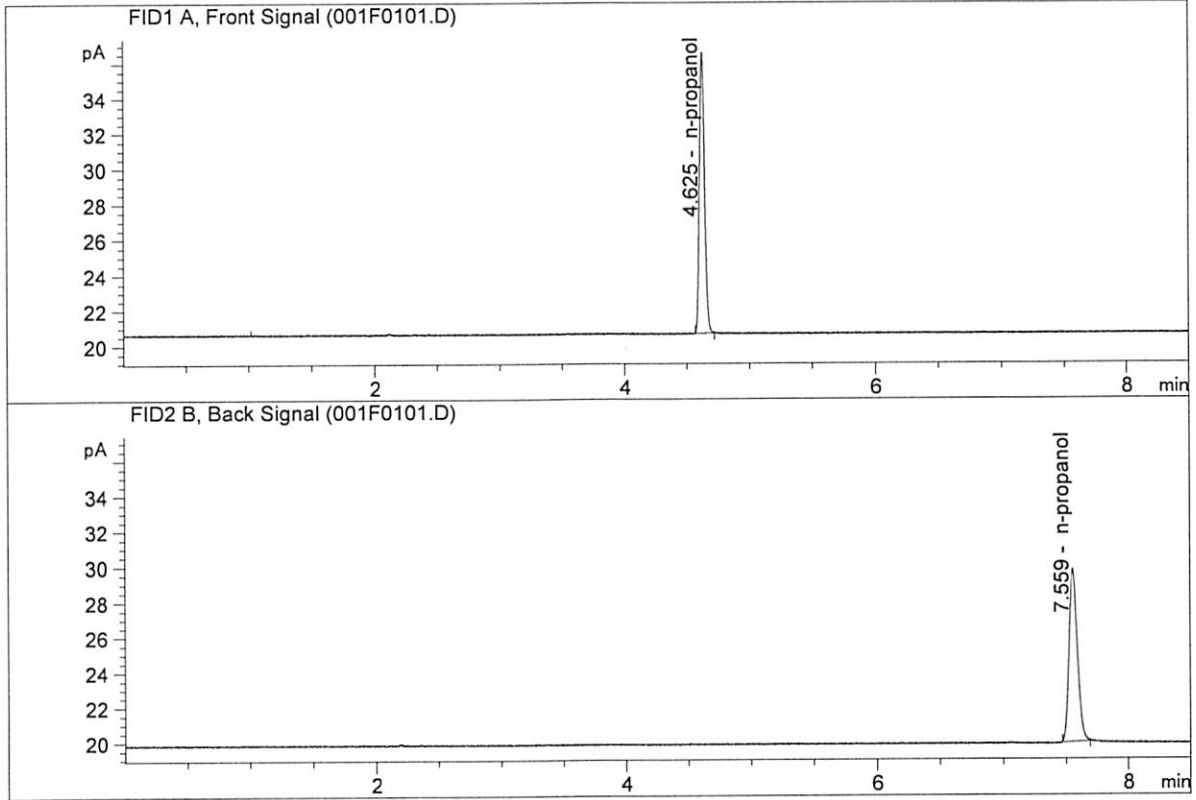

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	45.35698	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.24674	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report

Sample Name : MIX VOL FN06041502
 Laboratory : Meridian
 Injection Date : Jul 2, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

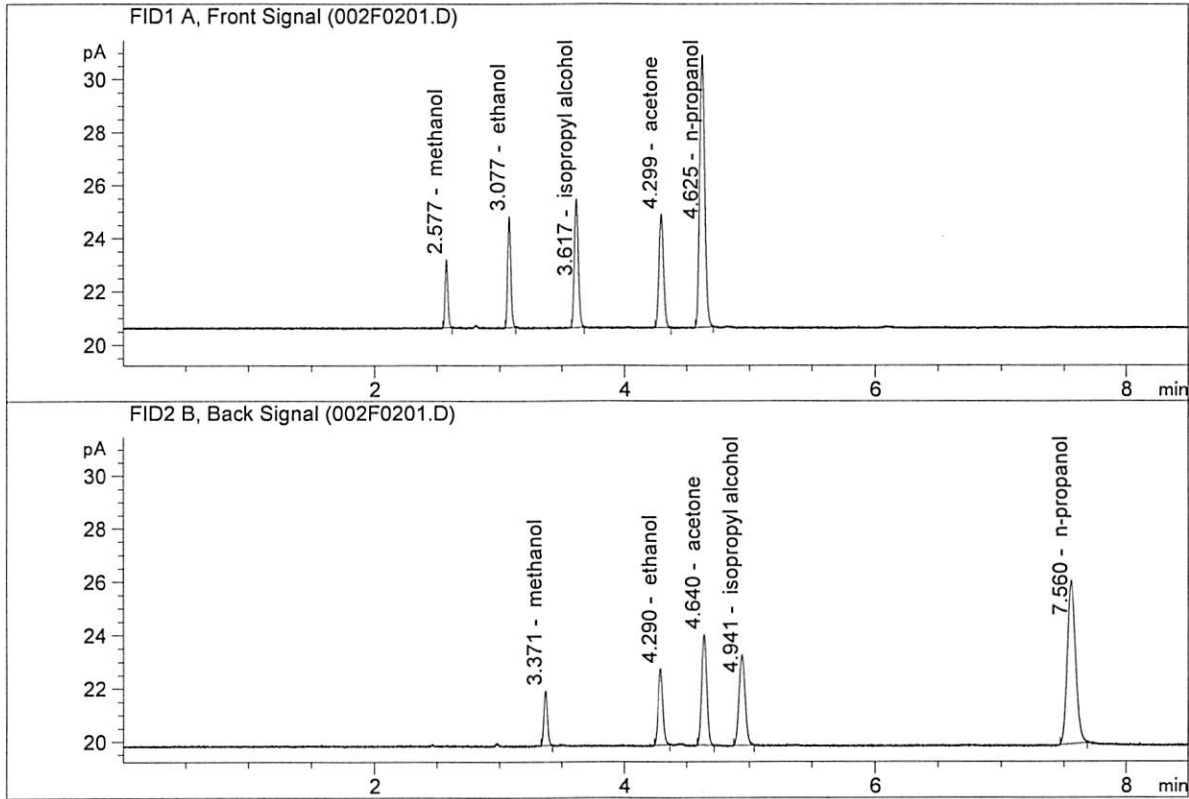

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.39441	0.1319	g/100cc
2.	Ethanol	Column 2:	7.67618	0.1339	g/100cc
3.	n-Propanol	Column 1:	28.88295	1.0000	g/100cc
4.	n-Propanol	Column 2:	29.41663	1.0000	g/100cc

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC1-1

Analysis Date(s): 02 Jul 2019

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.0799	0.0808	0.0009	0.0803	0.0803	
(g/100cc)	0.0799	0.0807	0.0008	0.0803		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: Alcohol.m
Hamilton Auto-Dilutor Serial Number: ML600HC11378

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.080	0.076	0.084	0.004


	Reported Result	
	0.080	

Calibration and control data are stored centrally.

16

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-1-A
 Laboratory : Meridian
 Injection Date : Jul 2, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

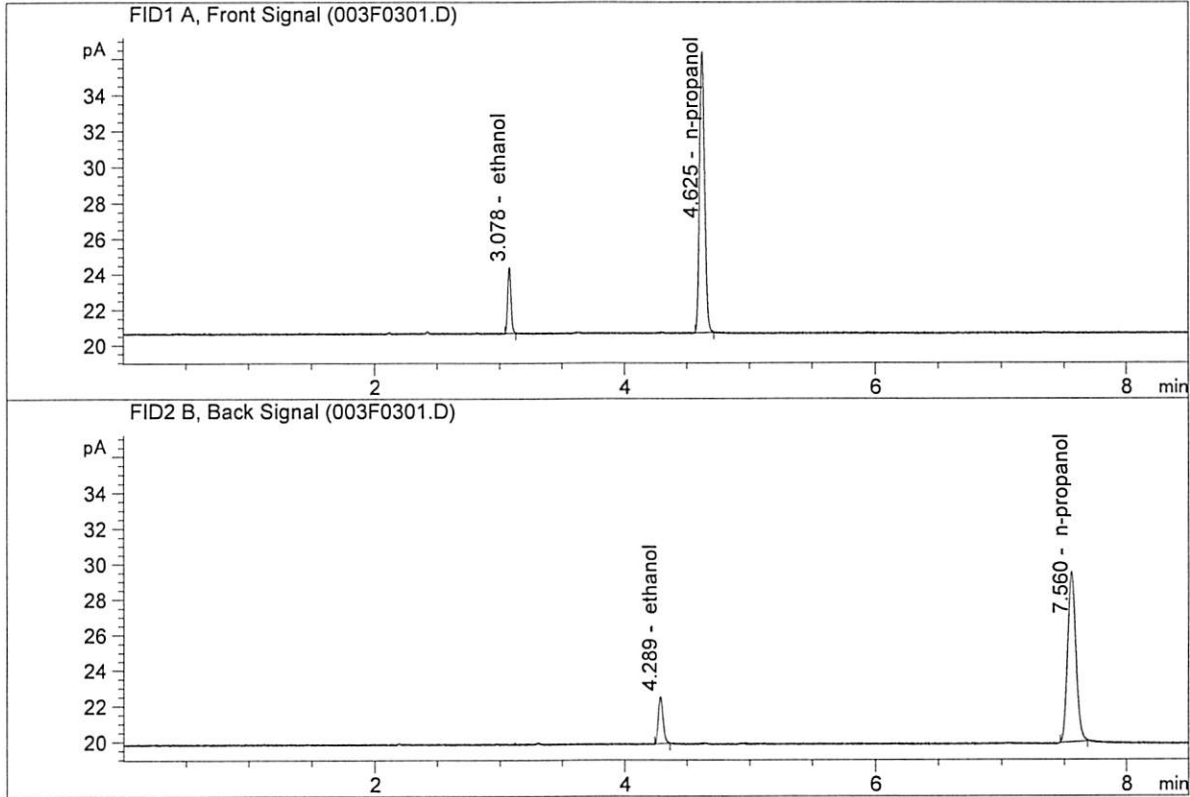


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	6.87636	0.0799	g/100cc
2.	Ethanol	Column 2:	7.07510	0.0808	g/100cc
3.	n-Propanol	Column 1:	44.67301	1.0000	g/100cc
4.	n-Propanol	Column 2:	46.16801	1.0000	g/100cc

JG

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-1-B
 Laboratory : Meridian
 Injection Date : Jul 2, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

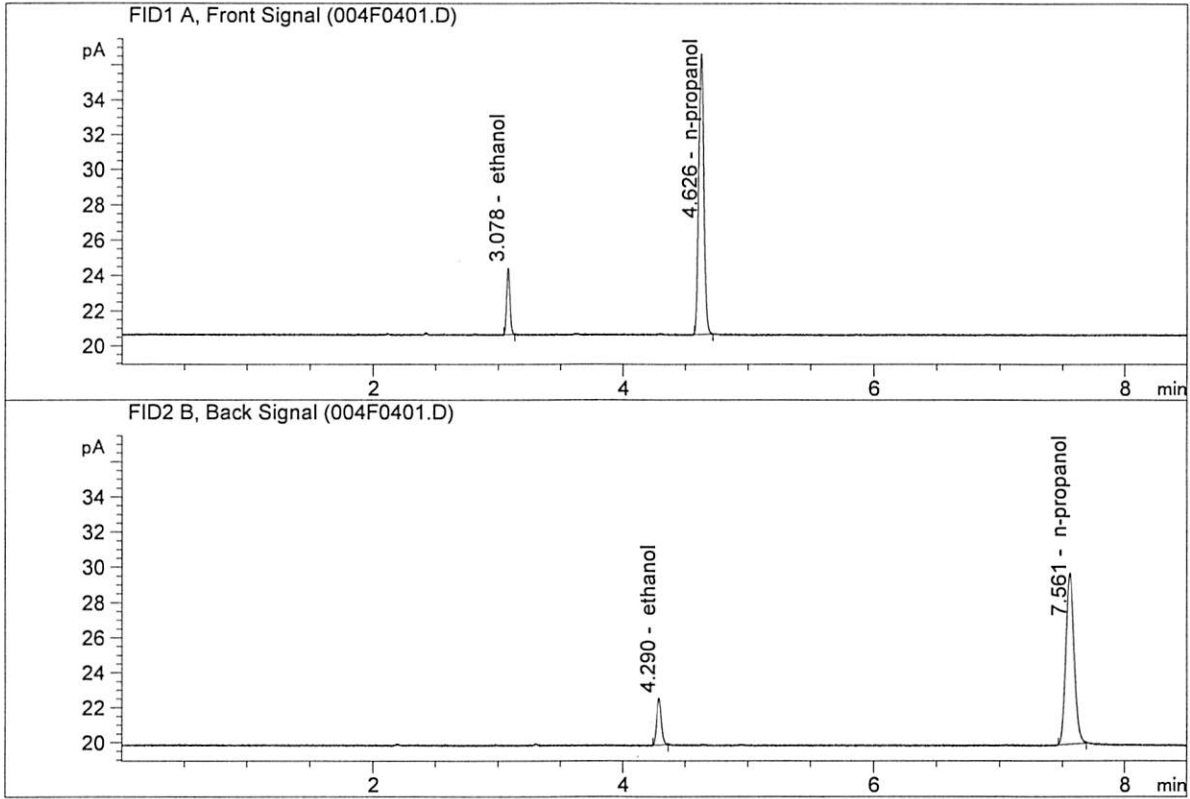

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.00782	0.0799	g/100cc
2.	Ethanol	Column 2:	7.20291	0.0807	g/100cc
3.	n-Propanol	Column 1:	45.49415	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.04325	1.0000	g/100cc

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: 0.08 FN04171701

Analysis Date(s): 02 Jul 2019

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.0805	0.0810	0.0005	0.0807	0.0806	
(g/100cc)	0.0804	0.0808	0.0004	0.0806		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: Alcohol.m
Hamilton Auto-Dilutor Serial Number: ML600HC11378

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.080	0.076	0.084	0.004

	Reported Result	
	0.080	

Calibration and control data are stored centrally.

Revision: 1


Issue Date: 01/04/2019

Issuing Authority: Quality Manager

JK

ISP Forensic Services Blood Alcohol Report


Sample Name : 0.08 FN04171701-A
 Laboratory : Meridian
 Injection Date : Jul 2, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

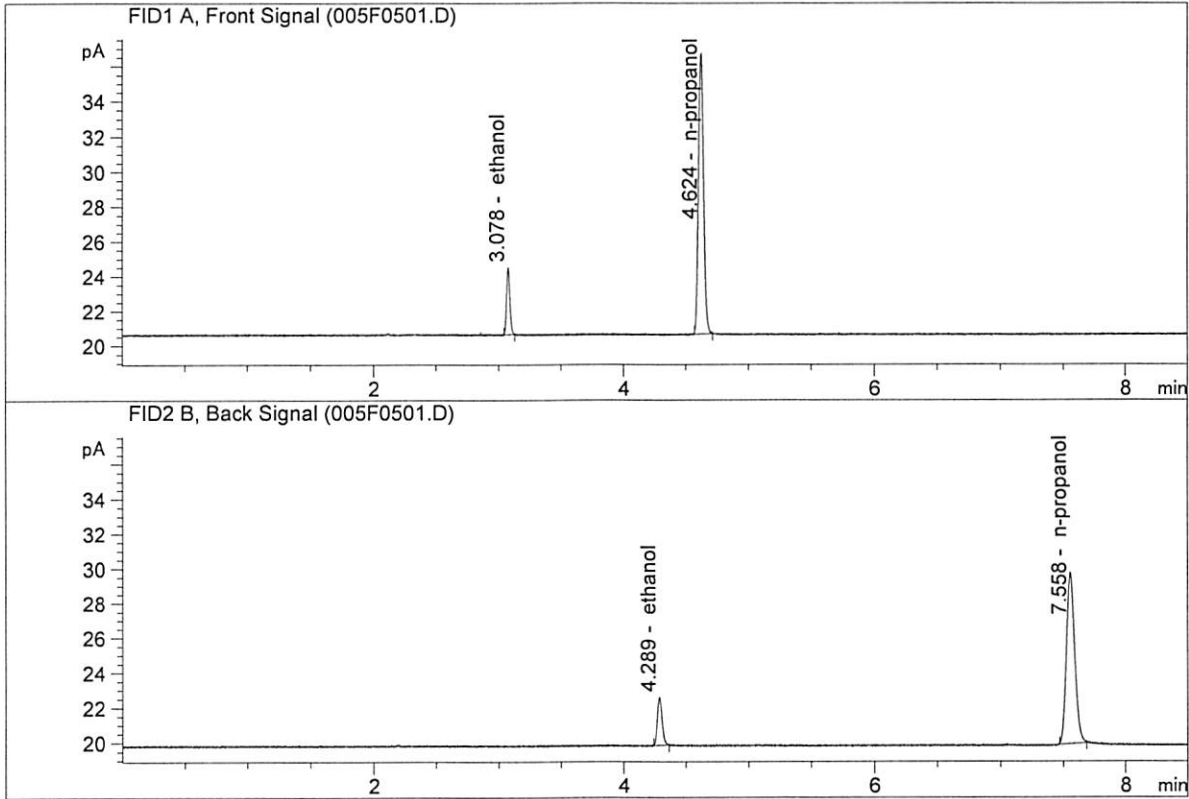

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.08973	0.0805	g/100cc
2.	Ethanol	Column 2:	7.27329	0.0810	g/100cc
3.	n-Propanol	Column 1:	45.73441	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.30840	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.08 FN04171701-B
 Laboratory : Meridian
 Injection Date : Jul 2, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

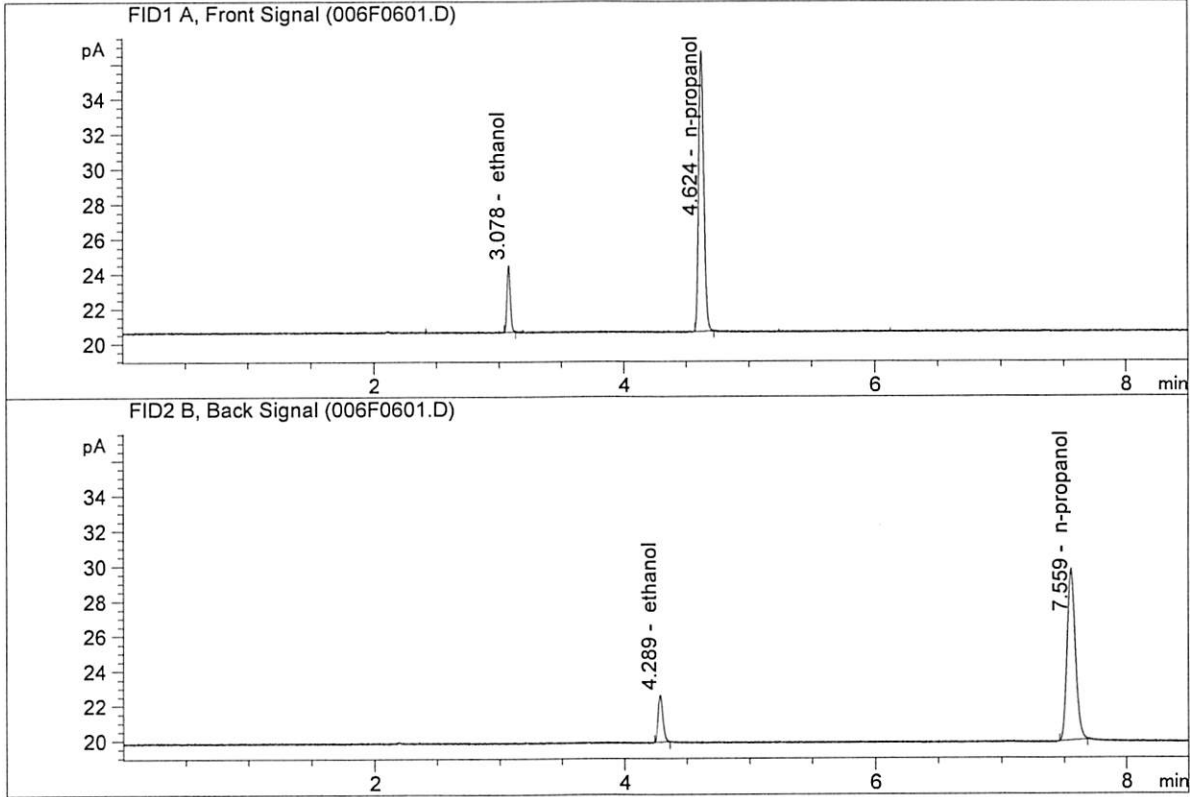

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.09197	0.0804	g/100cc
2.	Ethanol	Column 2:	7.24739	0.0808	g/100cc
3.	n-Propanol	Column 1:	45.75776	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.26926	1.0000	g/100cc

16

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC2-1

Analysis Date(s): 02 Jul 2019

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.2044	0.2043	0.0001	0.2043	0.2046	
(g/100cc)	0.2048	0.2049	0.0001	0.2048		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: Alcohol.m
Hamilton Auto-Dilutor Serial Number: ML600HC11378

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.204	0.193	0.215	0.011

	Reported Result	
	0.204	

Calibration and control data are stored centrally.

JG


Revision: 1

Issue Date: 01/04/2019

Issuing Authority: Quality Manager

ISP Forensic Services Blood Alcohol Report


Sample Name : QC2-1-A
 Laboratory : Meridian
 Injection Date : Jul 2, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

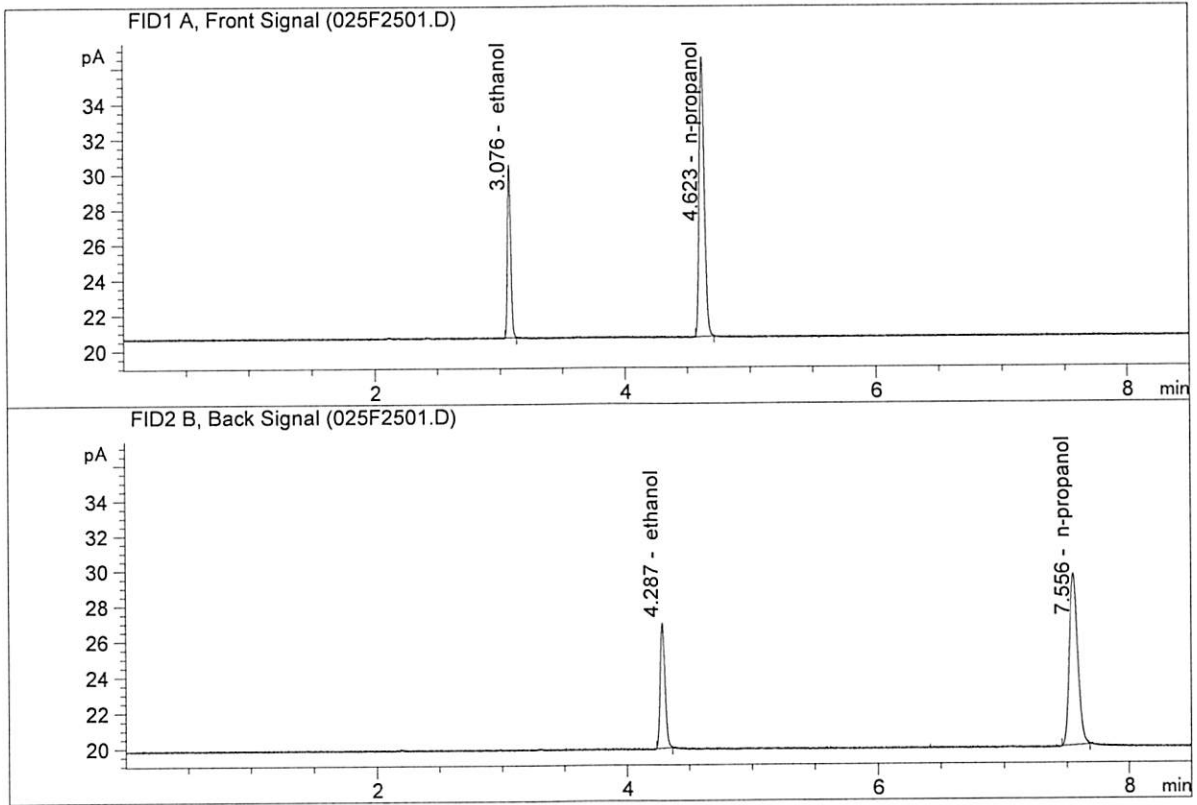

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	17.97301	0.2044	g/100cc
2.	Ethanol	Column 2:	18.66929	0.2043	g/100cc
3.	n-Propanol	Column 1:	45.14161	1.0000	g/100cc
4.	n-Propanol	Column 2:	46.27719	1.0000	g/100cc

ISP Forensic Services Blood Alcohol Report

Sample Name : QC2-1-B
 Laboratory : Meridian
 Injection Date : Jul 2, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

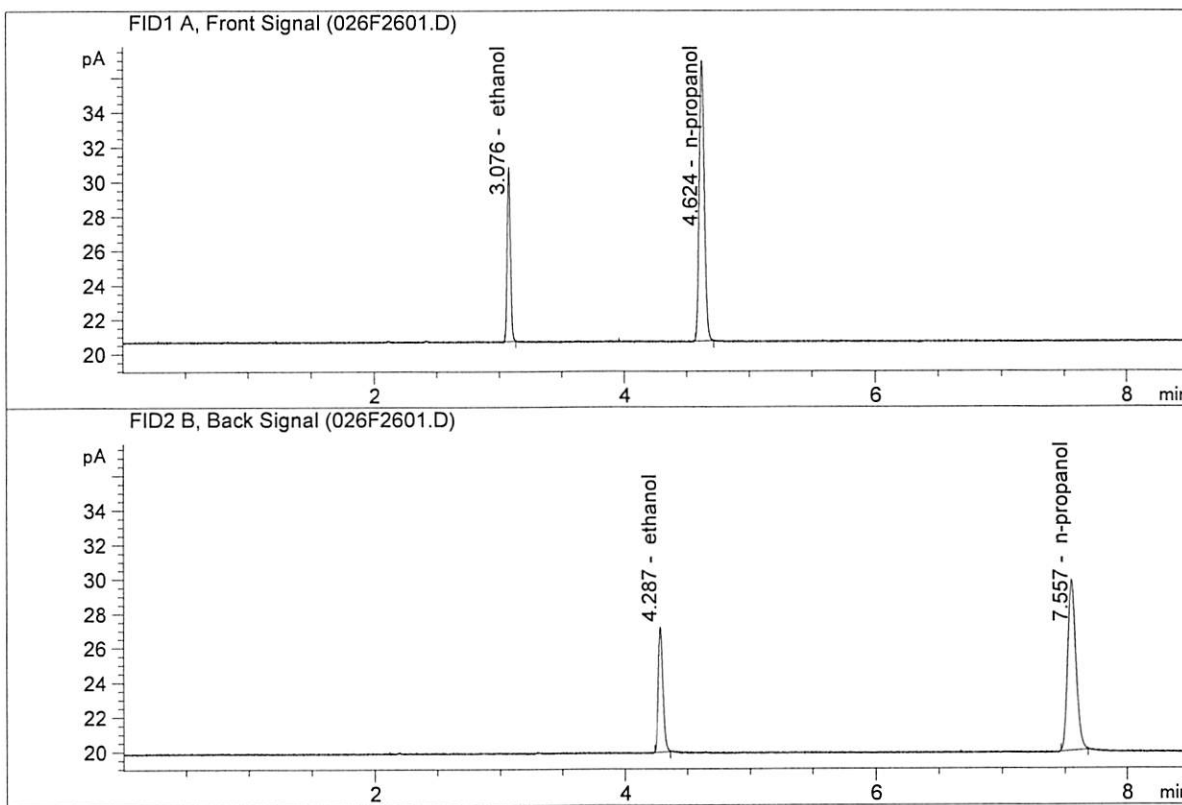

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	18.45100	0.2048	g/100cc
2.	Ethanol	Column 2:	19.20450	0.2049	g/100cc
3.	n-Propanol	Column 1:	46.25441	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.46056	1.0000	g/100cc

86

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC1-2

Analysis Date(s): 03 Jul 2019

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.0837	0.0846	0.0009	0.0841	0.0842	
(g/100cc)	0.0839	0.0849	0.0010	0.0844		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: Alcohol.m
Hamilton Auto-Dilutor Serial Number: ML600HC11378

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.084	0.079	0.089	0.005


	Reported Result	
	0.084	

Calibration and control data are stored centrally.

JK

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-2-A
 Laboratory : Meridian
 Injection Date : Jul 3, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

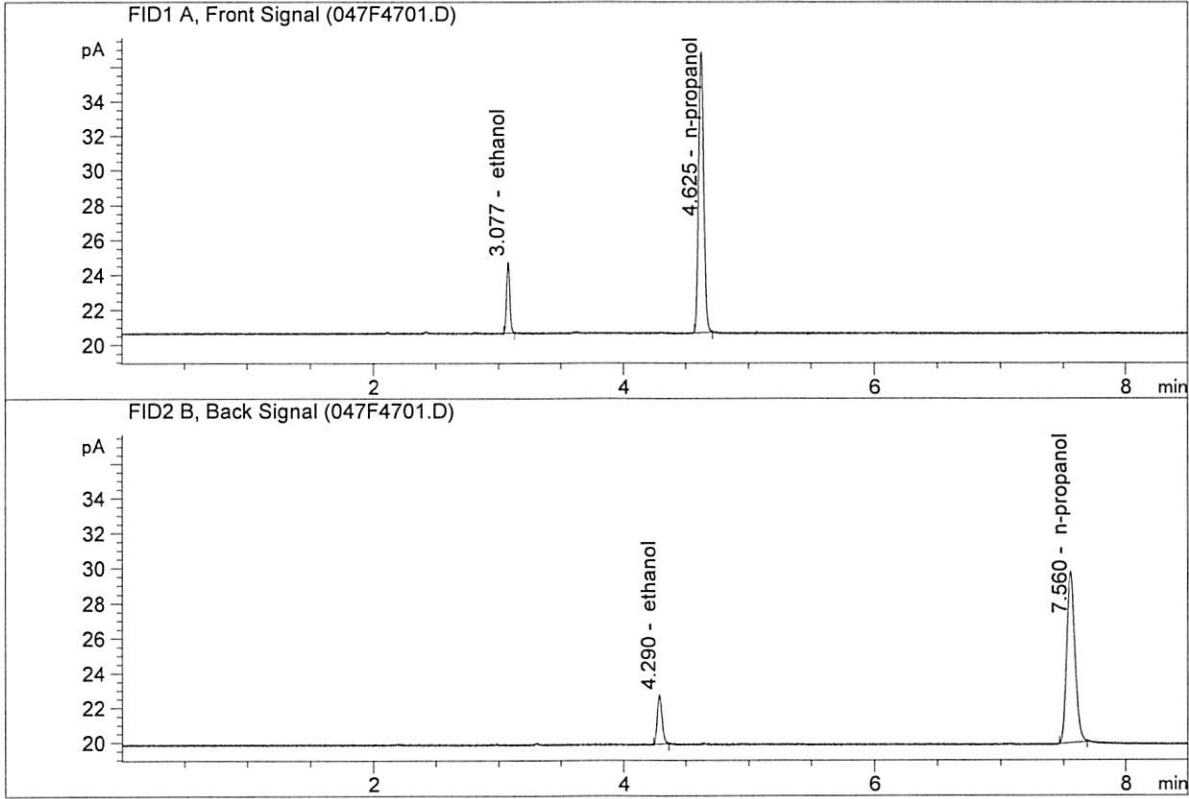


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.40544	0.0837	g/100cc
2.	Ethanol	Column 2:	7.57842	0.0846	g/100cc
3.	n-Propanol	Column 1:	45.88901	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.04196	1.0000	g/100cc

JG

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-2-B
 Laboratory : Meridian
 Injection Date : Jul 3, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

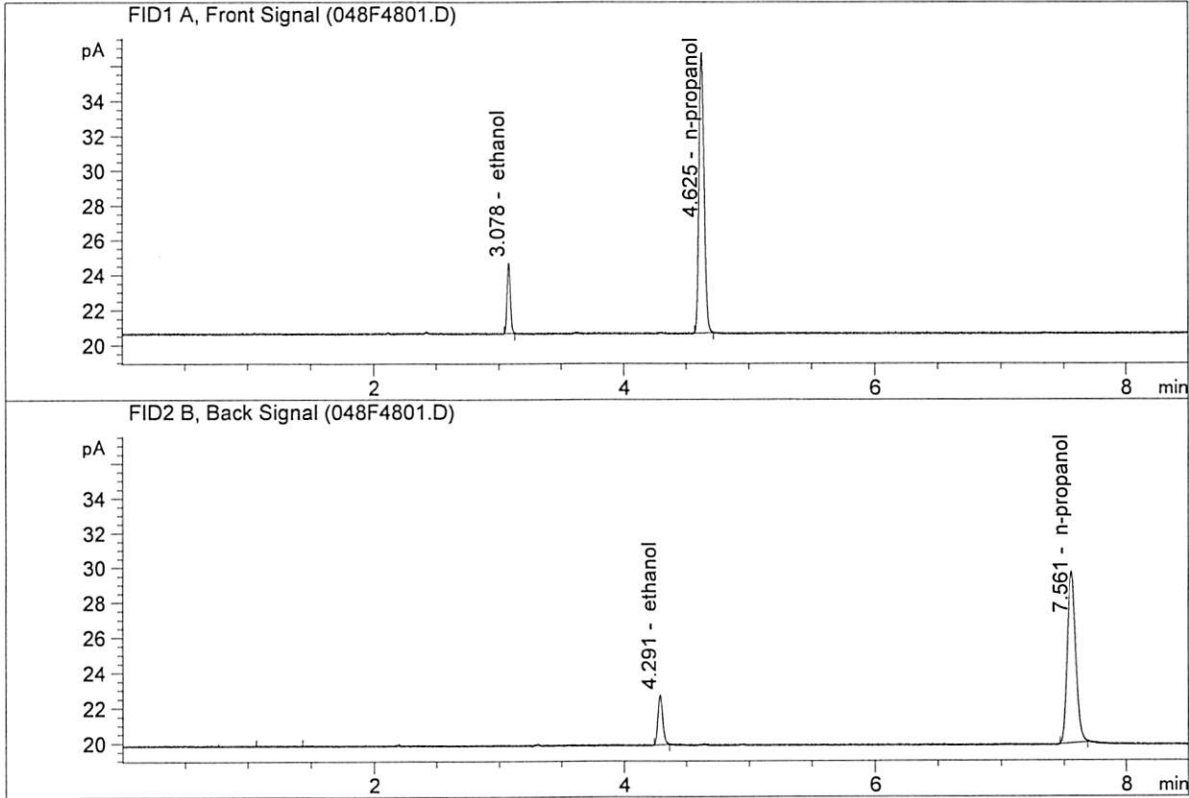


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.37960	0.0839	g/100cc
2.	Ethanol	Column 2:	7.54464	0.0849	g/100cc
3.	n-Propanol	Column 1:	45.60528	1.0000	g/100cc
4.	n-Propanol	Column 2:	46.66449	1.0000	g/100cc

JG

ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STD BLK
 Laboratory : Meridian
 Injection Date : Jul 3, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

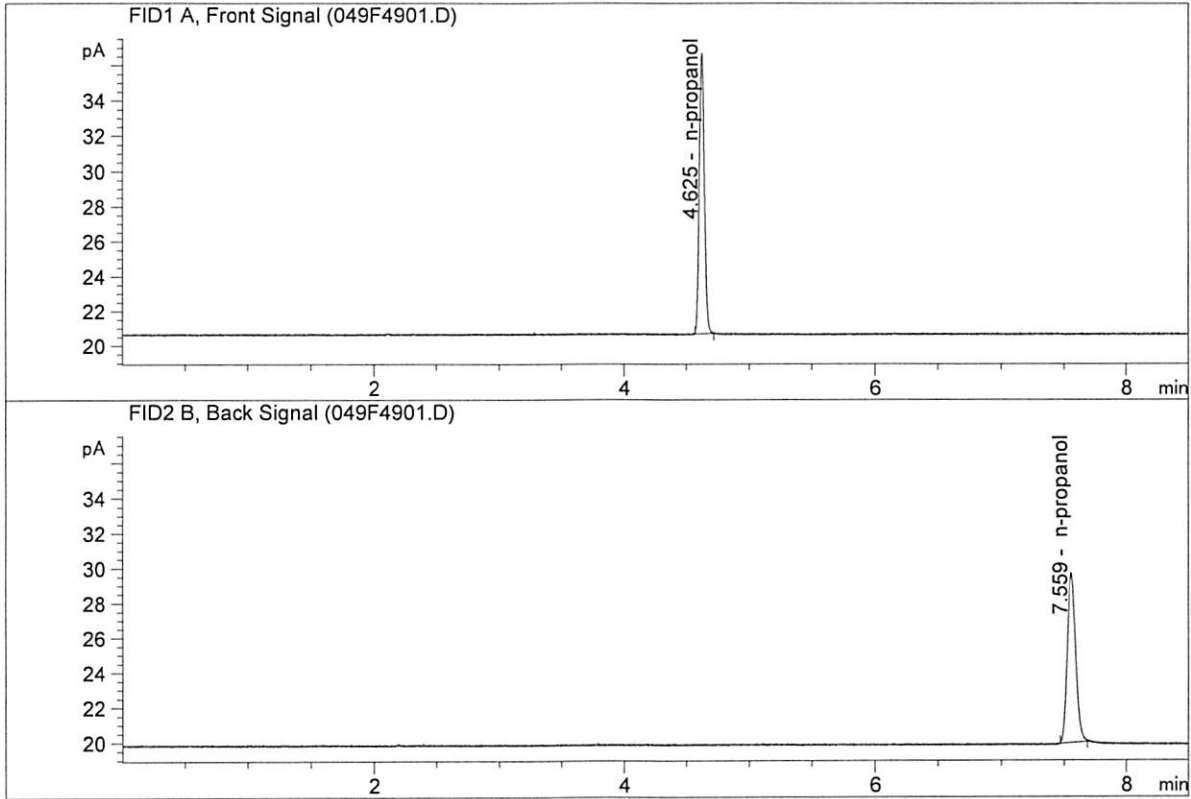

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	45.46254	1.0000	g/100cc
4.	n-Propanol	Column 2:	46.49068	1.0000	g/100cc

Sample Summary

Sequence table: C:\Chem32\1\Data\07-02-19_SAMPLES\07-02-19_SAMPLES 2019-07-02 16-44-39\07-02-19_SAMPLES.S
 Data directory path: C:\Chem32\1\Data\07-02-19_SAMPLES\07-02-19_SAMPLES 2019-07-02 16-44-39\
 Logbook: C:\Chem32\1\Data\07-02-19_SAMPLES\07-02-19_SAMPLES 2019-07-02 16-44-39\07-02-19_SAMPLES.LOG
 Sequence start: 7/2/2019 4:59:25 PM
 Sequence Operator: SYSTEM
 Operator: SYSTEM
 Method file name: C:\Chem32\1\Data\07-02-19_SAMPLES\07-02-19_SAMPLES 2019-07-02 16-44-39\ALCOHOL.M

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #	Cmp
1	1	1	INTERNAL STD BLK	-	1.0000	001F0101.D		2
2	2	1	MIX VOL FN060415	-	1.0000	002F0201.D		10
3	3	1	QC1-1-A	-	1.0000	003F0301.D		4
4	4	1	QC1-1-B	-	1.0000	004F0401.D		4
5	5	1	0.08 FN04171701-	-	1.0000	005F0501.D		4
6	6	1	0.08 FN04171701-	-	1.0000	006F0601.D		4
7	7	1	M2019-2773-1-A	-	1.0000	007F0701.D		4
8	8	1	M2019-2773-1-B	-	1.0000	008F0801.D		4
9	9	1	M2019-2774-1-A	-	1.0000	009F0901.D		4
10	10	1	M2019-2774-1-B	-	1.0000	010F1001.D		4
11	11	1	M2019-2775-1-A	-	1.0000	011F1101.D		4
12	12	1	M2019-2775-1-B	-	1.0000	012F1201.D		4
13	13	1	M2019-2776-1-A	-	1.0000	013F1301.D		4
14	14	1	M2019-2776-1-B	-	1.0000	014F1401.D		4
15	15	1	M2019-2783-1-A	-	1.0000	015F1501.D		4
16	16	1	M2019-2783-1-B	-	1.0000	016F1601.D		4
17	17	1	M2019-2859-1-A	-	1.0000	017F1701.D		2
18	18	1	M2019-2859-1-B	-	1.0000	018F1801.D		2
19	19	1	M2019-2860-1-A	-	1.0000	019F1901.D		4
20	20	1	M2019-2860-1-B	-	1.0000	020F2001.D		4
21	21	1	M2019-2870-1-A	-	1.0000	021F2101.D		2
22	22	1	M2019-2870-1-B	-	1.0000	022F2201.D		2
23	23	1	M2019-2882-1-A	-	1.0000	023F2301.D		4
24	24	1	M2019-2882-1-B	-	1.0000	024F2401.D		4
25	25	1	QC2-1-A	-	1.0000	025F2501.D		4
26	26	1	QC2-1-B	-	1.0000	026F2601.D		4
27	27	1	M2019-2908-1-A	-	1.0000	027F2701.D		4
28	28	1	M2019-2908-1-B	-	1.0000	028F2801.D		4
29	29	1	M2019-2909-1-A	-	1.0000	029F2901.D		4
30	30	1	M2019-2909-1-B	-	1.0000	030F3001.D		4
31	31	1	M2019-2944-1-A	-	1.0000	031F3101.D		4
32	32	1	M2019-2944-1-B	-	1.0000	032F3201.D		4
33	33	1	M2019-2981-1-A	-	1.0000	033F3301.D		4
34	34	1	M2019-2981-1-B	-	1.0000	034F3401.D		4
35	35	1	M2019-2998-1-A	-	1.0000	035F3501.D		4
36	36	1	M2019-2998-1-B	-	1.0000	036F3601.D		4
37	37	1	M2019-2999-1-A	-	1.0000	037F3701.D		4
38	38	1	M2019-2999-1-B	-	1.0000	038F3801.D		4
39	39	1	M2019-3000-1-A	-	1.0000	039F3901.D		4
40	40	1	M2019-3000-1-B	-	1.0000	040F4001.D		4
41	41	1	M2019-3001-1-A	-	1.0000	041F4101.D		4
42	42	1	M2019-3001-1-B	-	1.0000	042F4201.D		4
43	43	1	M2019-3002-1-A	-	1.0000	043F4301.D		2

JK

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #	# Cmp
44	44	1	M2019-3002-1-B	-	1.0000	044F4401.D		2
45	45	1	M2019-3002-2-A	-	1.0000	045F4501.D		2
46	46	1	M2019-3002-2-B	-	1.0000	046F4601.D		2
47	47	1	QC1-2-A	-	1.0000	047F4701.D		4
48	48	1	QC1-2-B	-	1.0000	048F4801.D		4
49	49	1	INTERNAL STD BLK	-	1.0000	049F4901.D		2

Method file name: C:\Chem32\1\Data\07-02-19_SAMPLES\07-02-19_SAMPLES 2019-07-02 16-44-39
 \SHUTDOWN.M

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #	# Cmp
50	50	1	EMPTY	-	1.0000	050F5001.D		0

JK