

Quantitative Analysis for Ethanol & Qualitative Analysis for Other Volatiles

Analytical Method(s): 1.0

Device: Hamilton MICROLAB 503A Liquid Processor/Dilutor Serial Number: ML600HC11378

Volatiles Quality Assurance Controls

Run Date(s): 09/12/2019

Calibration Date: 09/12/2019

Control level	Expiration	Lot #	Target Value	Acceptable Range	Overall Results
Level 1	Jan-22	1801036	0.0812	0.0731-0.0893	0.0793 g/100cc 0.0833 g/100cc g/100cc
Level 2	Mar-22	1803028	0.2035	0.1832-0.2238	0.2038 g/100cc 0.2026 g/100cc g/100cc
Multi-Component mixture:		Lot #	FN06041502		OK
Curve Fit:		Column 1	1.0000	Column 2	0.99997




















Ethanol Calibration Reference Material

Calibrator level	Target Value	Acceptable Range	Column 1	Column 2	Precision	Mean
50	0.050	0.045 - 0.055	0.0501	0.0514	0.0013	0.0507
100	0.100	0.090 - 0.110	0.0998	0.1000	0.0002	0.0999
200	0.200	0.180 - 0.220	0.2000	0.1988	0.0012	0.1994
300	0.300	0.270 - 0.330	0.3000	0.2986	0.0014	0.2993
500	0.500	0.450 - 0.550	0.5000	0.5012	0.0012	0.5006

Aqueous Controls

Control level	Target Value	Acceptable Range	Overall Results
80	0.080	0.076 - 0.084	0.080 g/100cc

Worklist: 3681

<u>LAB CASE</u>	<u>ITEM</u>	<u>TASK ID</u>	<u>DESCRIPTION</u>	
M2019-3926	1	161950	Alcohol Analysis	
M2019-3927	1	161951	Alcohol Analysis	
M2019-3934	1	162015	Alcohol Analysis	
M2019-3935	1	162016	Alcohol Analysis	
M2019-3940	1	162047	Alcohol Analysis	
M2019-3954	1	162185	Alcohol Analysis	
M2019-3955	1	162186	Alcohol Analysis	
M2019-3962	1	162376	Alcohol Analysis	
M2019-3972	2	162401	Alcohol Analysis	
M2019-3974	1	162433	Alcohol Analysis	
M2019-3975	1	162437	Alcohol Analysis	
M2019-3976	1	162441	Alcohol Analysis	
M2019-3977	1	162445	Alcohol Analysis	
M2019-3991	1	162468	Alcohol Analysis	
M2019-3991	2	162469	Alcohol Analysis	
M2019-4017	1	162596	Alcohol Analysis	
M2019-4065	1	162964	Alcohol Analysis	
M2019-4066	1	162965	Alcohol Analysis	
M2019-4110	1	163211	Alcohol Analysis	
M2019-4112	1	163213	Alcohol Analysis	

fr

=====
Calibration Table
=====

General Calibration Setting

Calib. Data Modified : Thursday, September 12, 2019 9:59:49 AM
Signals calculated separately : No

Rel. Reference Window : 0.000 %
Abs. Reference Window : 0.100 min
Rel. Non-ref. Window : 0.000 %
Abs. Non-ref. Window : 0.100 min
Uncalibrated Peaks : not reported
Partial Calibration : Yes, identified peaks are recalibrated
Correct All Ret. Times: No, only for identified peaks

Curve Type : Linear
Origin : Ignored
Weight : Equal

Recalibration Settings:
Average Response : Average all calibrations
Average Retention Time: Floating Average New 75%

Calibration Report Options :
Printout of recalibrations within a sequence:
 Calibration Table after Recalibration
 Normal Report after Recalibration
If the sequence is done with bracketing:
 Results of first cycle (ending previous bracket)

Default Sample ISTD Information (if not set in sample table):

ISTD #	ISTD Amount [g/100cc]	Name
1	1.00000	n-propanol
2	1.00000	n-propanol

Signal Details

Signal 1: FID1 A, Front Signal
Signal 2: FID2 B, Back Signal

Overview Table

55

RT	Sig	Lvl	Amount [g/100cc]	Area	Rsp.Factor	Ref	ISTD #	Compound
2.586	1	1	1.00000	3.69669	2.70512e-1	No	No 1	methanol
2.809	1	1	1.00000	4.26100	2.34687e-1	No	No 2	Acetaldehyde
2.977	2	1	1.00000	4.26100	2.34687e-1	No	No 2	Acetaldehyde
3.075	1	1	5.00000e-2	4.38270	1.14085e-2	No	No 1	ethanol
		2	1.00000e-1	8.64185	1.15716e-2			
		3	2.00000e-1	17.47327	1.14461e-2			
		4	3.00000e-1	26.32771	1.13948e-2			
		5	5.00000e-1	44.15454	1.13239e-2			
3.388	2	1	1.00000	4.26062	2.34707e-1	No	No 2	methanol
3.628	1	1	1.00000	9.73055	1.02769e-1	No	No 1	isopropyl alcohol
4.285	2	1	5.00000e-2	4.50800	1.10914e-2	No	No 2	ethanol
		2	1.00000e-1	8.94254	1.11825e-2			
		3	2.00000e-1	18.16210	1.10119e-2			
		4	3.00000e-1	27.48956	1.09132e-2			
		5	5.00000e-1	46.59861	1.07299e-2			
4.308	1	1	1.00000	6.49940	1.53860e-1	No	No 1	acetone
4.620	1	1	1.00000	46.08063	2.17011e-2	No	Yes 1	n-propanol
		2	1.00000	45.04212	2.22014e-2			
		3	1.00000	45.15342	2.21467e-2			
		4	1.00000	45.26142	2.20939e-2			
		5	1.00000	45.47670	2.19893e-2			
4.661	2	1	1.00000	6.89301	1.45075e-1	No	No 2	acetone
4.969	2	1	1.00000	10.70642	9.34019e-2	No	No 2	isopropyl alcohol
7.550	2	1	1.00000	48.27920	2.07129e-2	No	Yes 2	n-propanol
		2	1.00000	46.85571	2.13421e-2			
		3	1.00000	46.68904	2.14183e-2			
		4	1.00000	46.67542	2.14246e-2			
		5	1.00000	46.82527	2.13560e-2			


Peak Sum Table

No Entries in table

1 Warnings or Errors :


Warning : Curve requires more calibration points., (methanol)

Calibration Curves

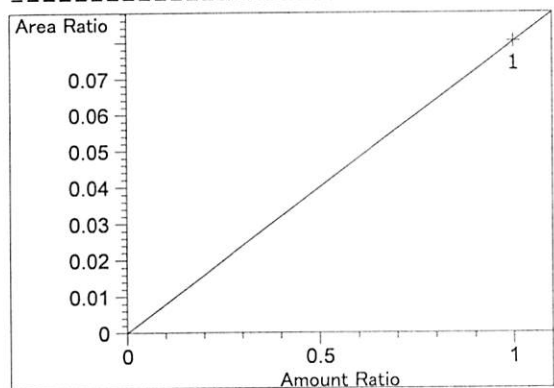


methanol at exp. RT: 2.586
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 8.02223e-2
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio


SV

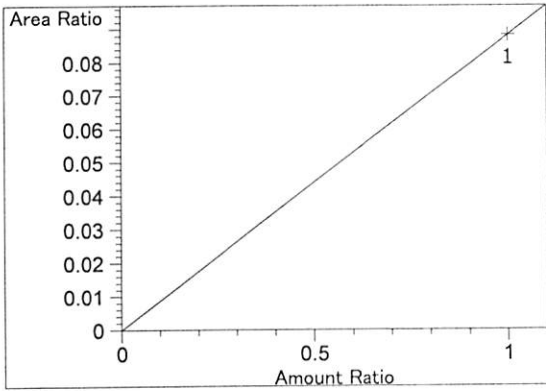


Acetaldehyde at exp. RT: 2.809
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 8.82575e-2
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio

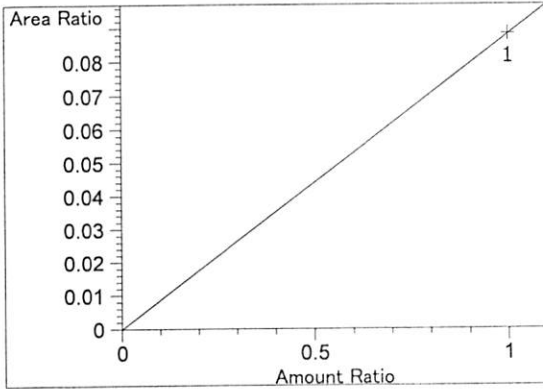

Acetaldehyde at exp. RT: 2.977
 FID2 B, Back Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 8.82575e-2
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio

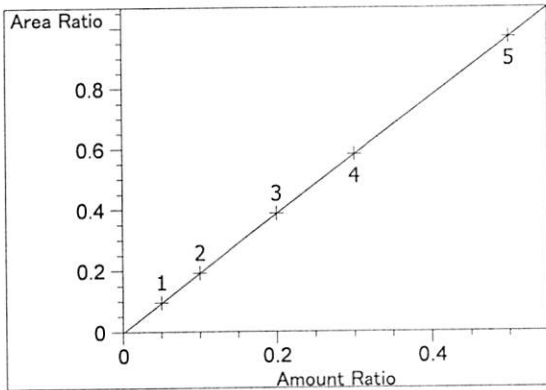


ethanol at exp. RT: 3.075
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00026
 Formula: $y = mx + b$
 m: 1.94685
 b: -2.46488e-3
 x: Amount Ratio
 y: Area Ratio

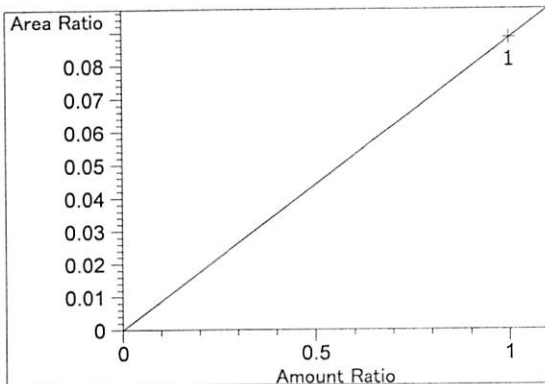


methanol at exp. RT: 3.388
 FID2 B, Back Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 8.82497e-2
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio


fr

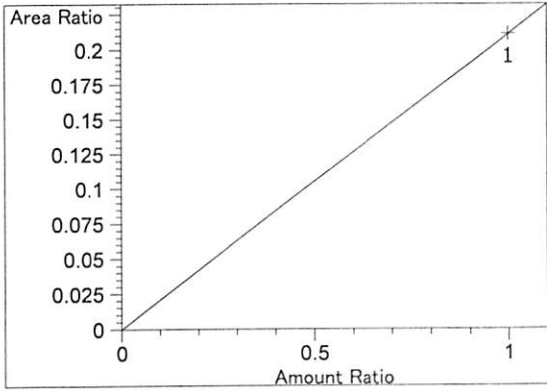


isopropyl alcohol at exp. RT: 3.628
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 2.11164e-1
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio

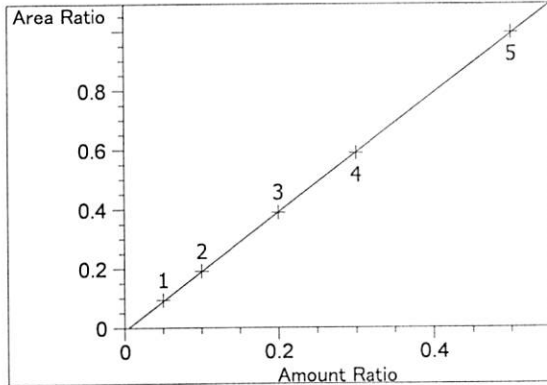

ethanol at exp. RT: 4.285
 FID2 B, Back Signal
 Correlation: 0.99997
 Residual Std. Dev.: 0.00300
 Formula: $y = mx + b$
 m: 2.00493
 b: -9.66698e-3
 x: Amount Ratio
 y: Area Ratio

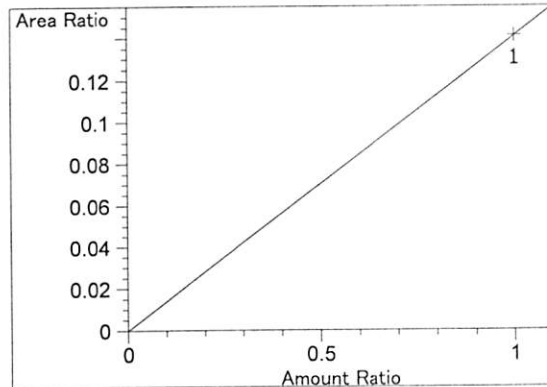


acetone at exp. RT: 4.308
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 1.41044e-1
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio

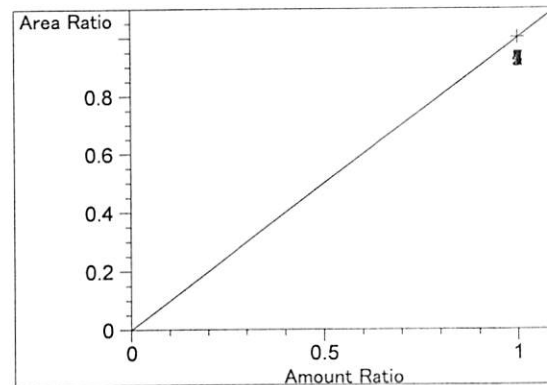


n-propanol at exp. RT: 4.620
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 1.00000
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio


BR

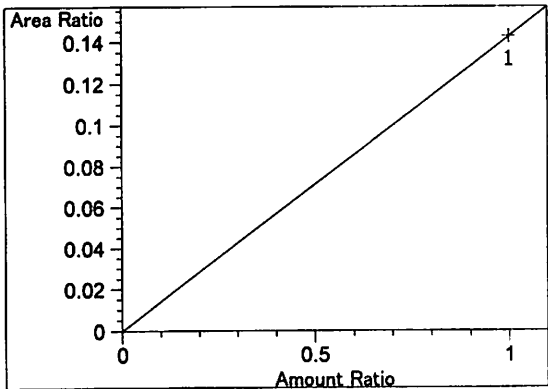

acetone at exp. RT: 4.661
FID2 B, Back Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx + b$
m: 1.42774e-1
b: 0.00000
x: Amount Ratio
y: Area Ratio

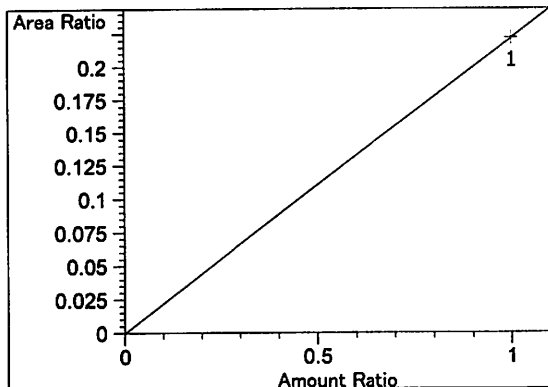

isopropyl alcohol at exp. RT: 4.969
FID2 B, Back Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx + b$
m: 2.21760e-1
b: 0.00000
x: Amount Ratio
y: Area Ratio

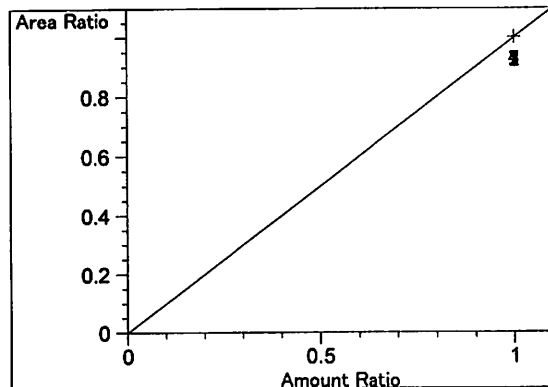

n-propanol at exp. RT: 7.550
FID2 B, Back Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx + b$
m: 1.00000
b: 0.00000
x: Amount Ratio
y: Area Ratio

=====

W

S a m p l e S u m m a r y


Sequence table: C:\Chem32\1\Data\09-12-19_CAL\09-12-19_CAL 2019-09-12 08-54-39\09-12-19_CAL.S
 Data directory path: C:\Chem32\1\Data\09-12-19_CAL\09-12-19_CAL 2019-09-12 08-54-39\
 Logbook: C:\Chem32\1\Data\09-12-19_CAL\09-12-19_CAL 2019-09-12 08-54-39\09-12-19_CAL.LOG
 Sequence start: 9/12/2019 9:09:17 AM
 Sequence Operator: SYSTEM
 Operator: SYSTEM

Method file name: C:\Chem32\1\Data\09-12-19_CAL\09-12-19_CAL 2019-09-12 08-54-39\ALCOHOL.M

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #	# Cmp
1	1	1	0.050 FN05211804	-	1.0000	001F0101.D	*	4
2	2	1	0.100 FN02271802	-	1.0000	002F0201.D	*	4
3	3	1	0.200 FN06231704	-	1.0000	003F0301.D	*	4
4	4	1	0.300 FN07311804	-	1.0000	004F0401.D	*	4
5	5	1	0.500 FN08031602	-	1.0000	005F0501.D	*	4
6	6	1	INTERNAL STANDAR	-	1.0000	006F0601.D		2

ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STANDARD BLANK
 Laboratory : Meridian
 Injection Date : Sep 12, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

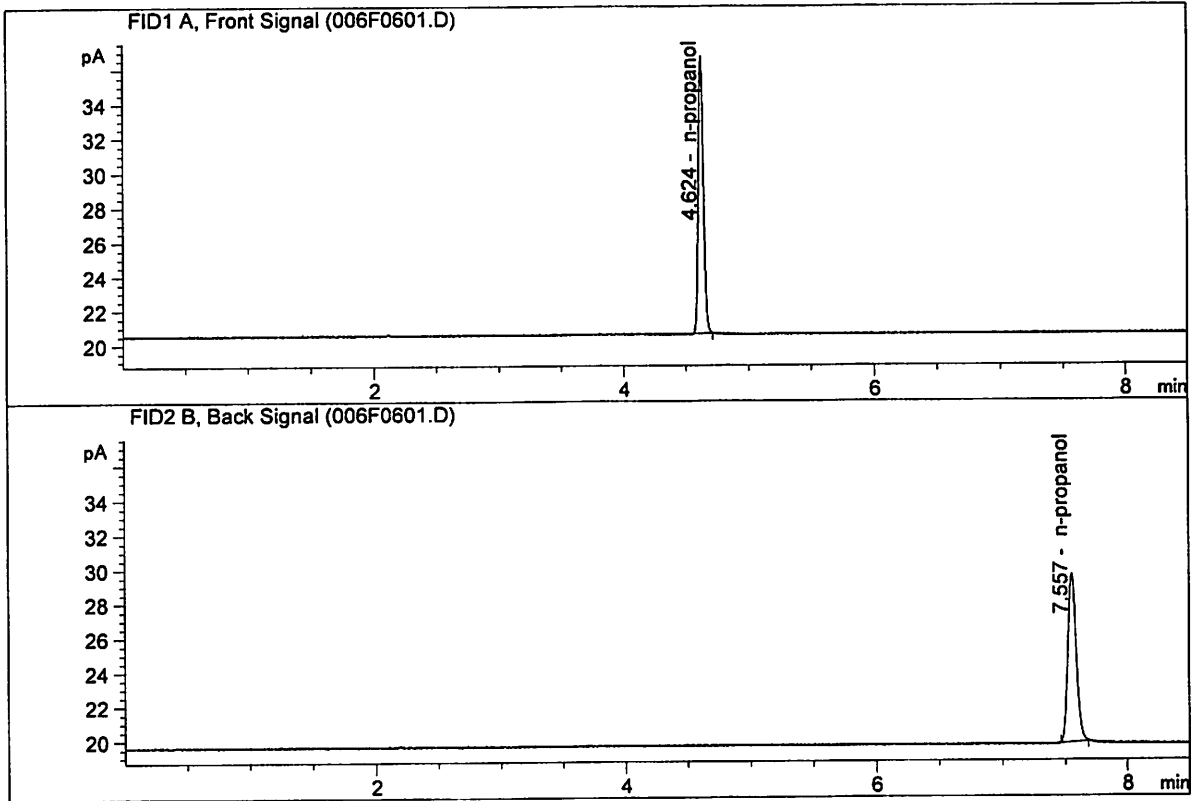


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	45.79055	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.26173	1.0000	g/100cc

65

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.050 FN05211804
 Laboratory : Meridian
 Injection Date : Sep 12, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

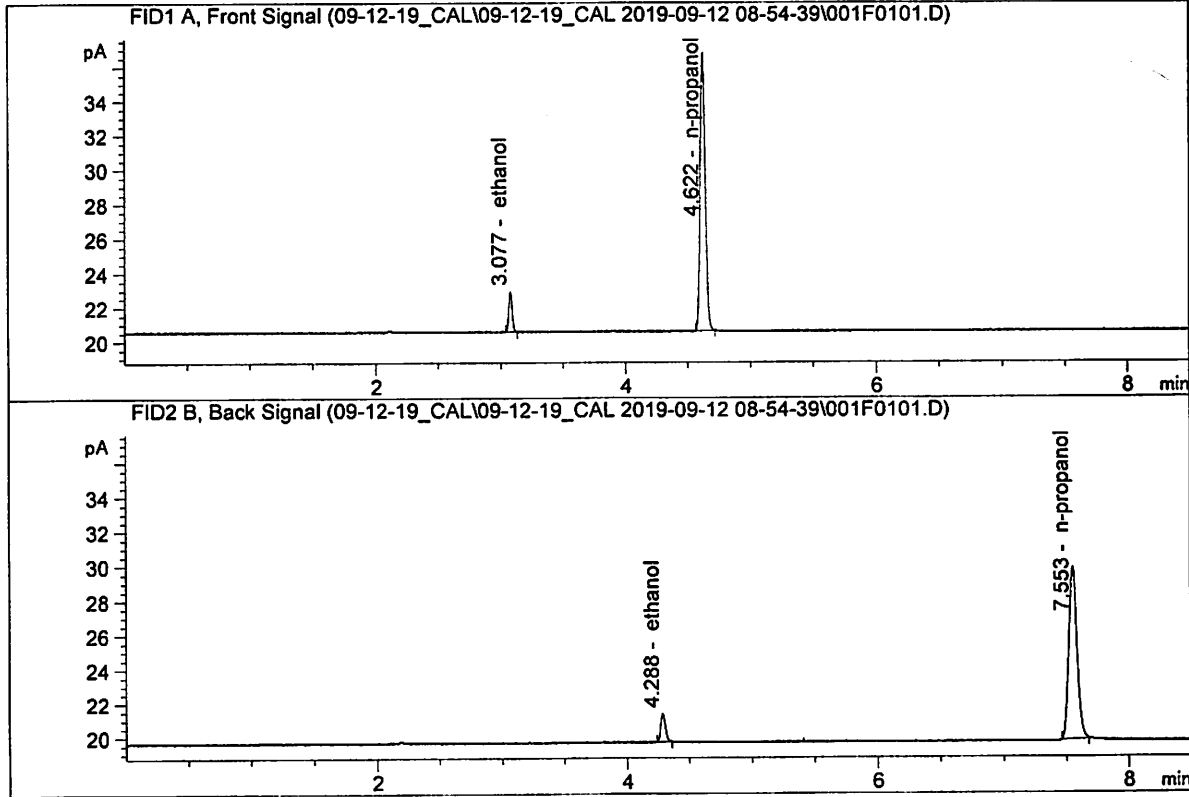


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	4.38270	0.0501	g/100cc
2.	Ethanol	Column 2:	4.50800	0.0514	g/100cc
3.	n-Propanol	Column 1:	46.08063	1.0000	g/100cc
4.	n-Propanol	Column 2:	48.27920	1.0000	g/100cc

68

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.100 FN02271802
 Laboratory : Meridian
 Injection Date : Sep 12, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

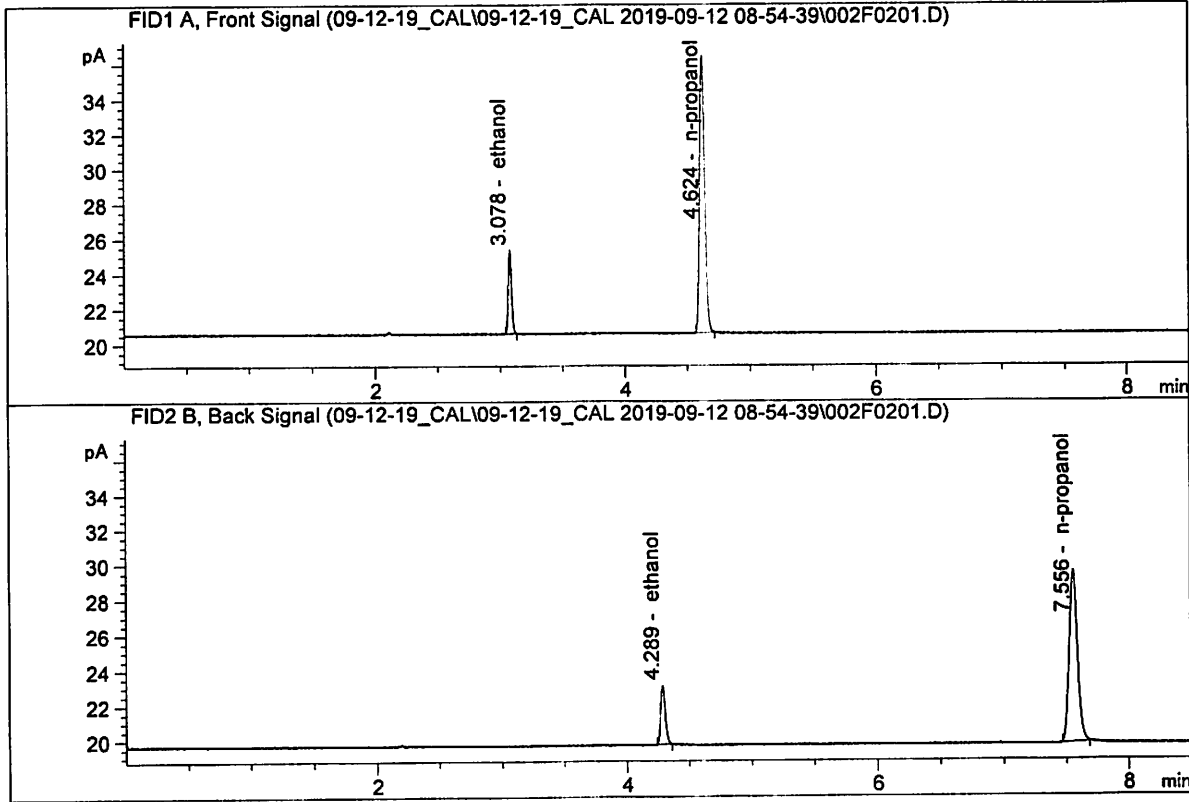


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	8.64185	0.0998	g/100cc
2.	Ethanol	Column 2:	8.94254	0.1000	g/100cc
3.	n-Propanol	Column 1:	45.04212	1.0000	g/100cc
4.	n-Propanol	Column 2:	46.85571	1.0000	g/100cc

62

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.200 FN06231704
 Laboratory : Meridian
 Injection Date : Sep 12, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

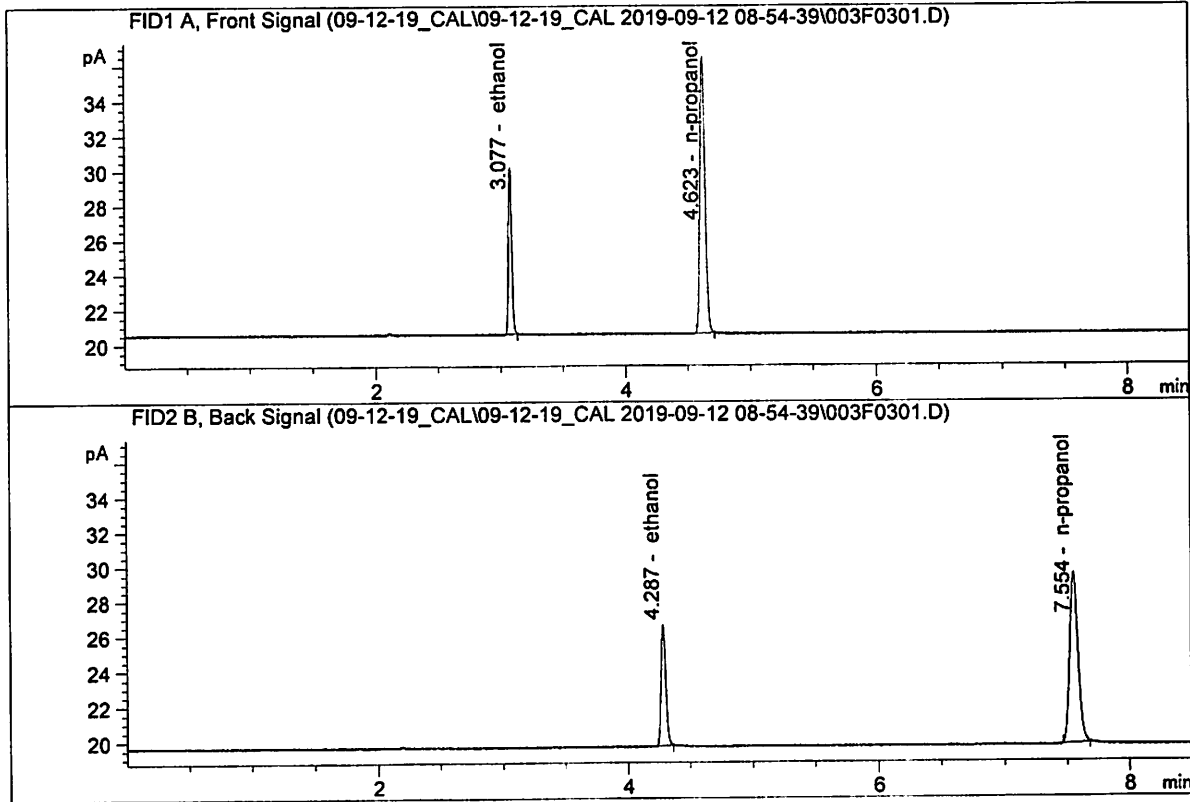


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	17.47327	0.2000	g/100cc
2.	Ethanol	Column 2:	18.16210	0.1988	g/100cc
3.	n-Propanol	Column 1:	45.15342	1.0000	g/100cc
4.	n-Propanol	Column 2:	46.68904	1.0000	g/100cc

60

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.300 FN07311804
 Laboratory : Meridian
 Injection Date : Sep 12, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

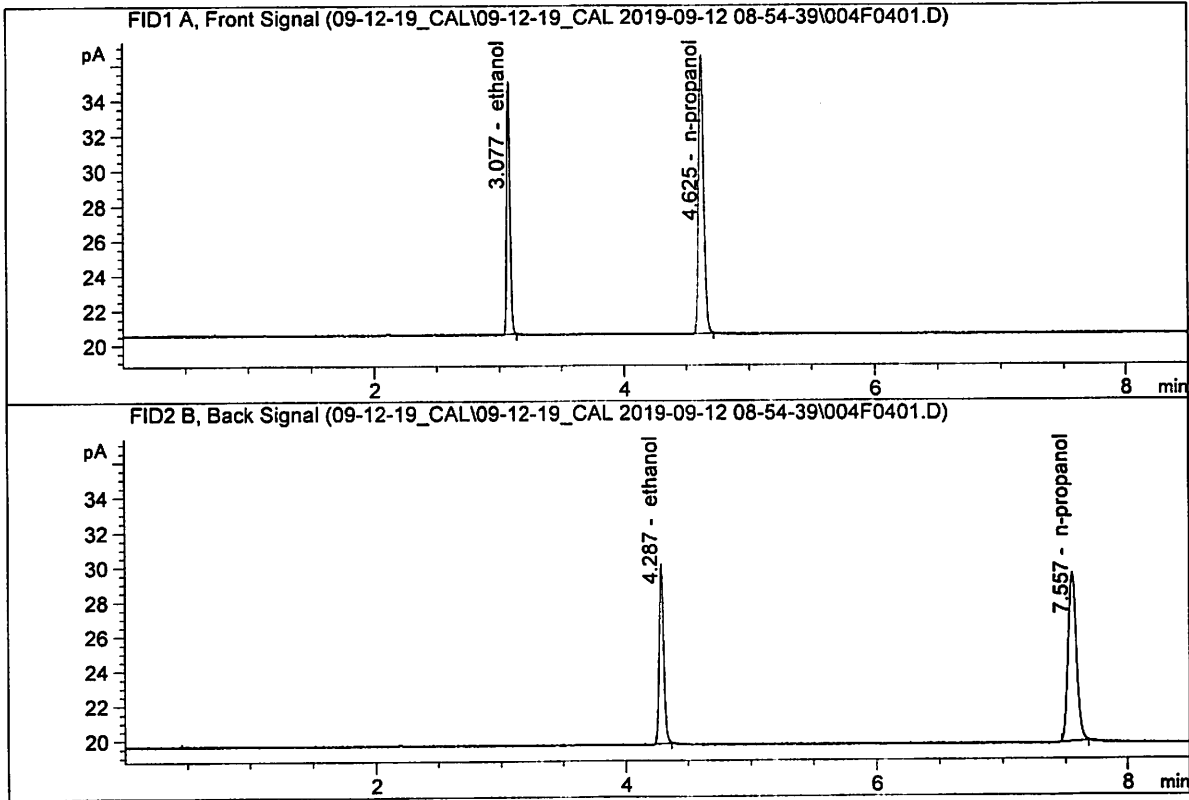


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	26.32771	0.3000	g/100cc
2.	Ethanol	Column 2:	27.48956	0.2986	g/100cc
3.	n-Propanol	Column 1:	45.26142	1.0000	g/100cc
4.	n-Propanol	Column 2:	46.67542	1.0000	g/100cc

62

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.500 FN08031602
 Laboratory : Meridian
 Injection Date : Sep 12, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

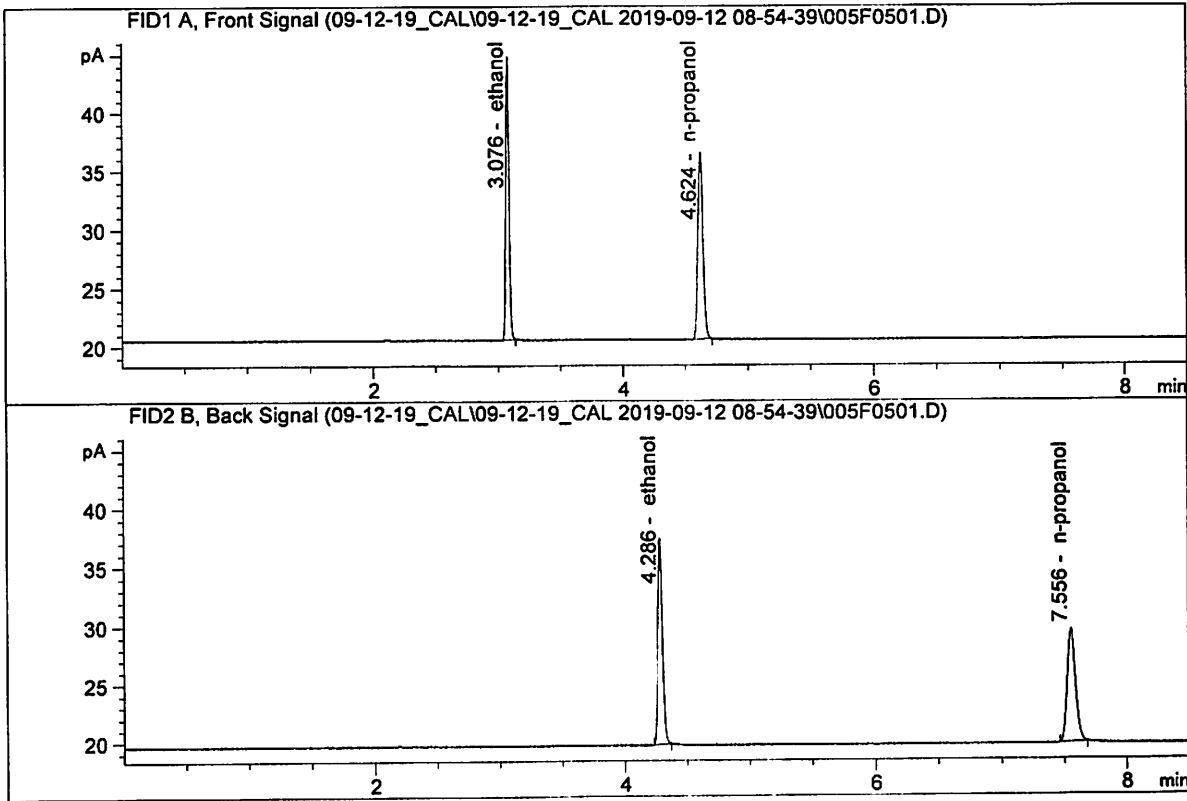


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	44.15454	0.5000	g/100cc
2.	Ethanol	Column 2:	46.59861	0.5012	g/100cc
3.	n-Propanol	Column 1:	45.47670	1.0000	g/100cc
4.	n-Propanol	Column 2:	46.82527	1.0000	g/100cc

15

ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STD BLK 1
 Laboratory : Meridian
 Injection Date : Sep 12, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

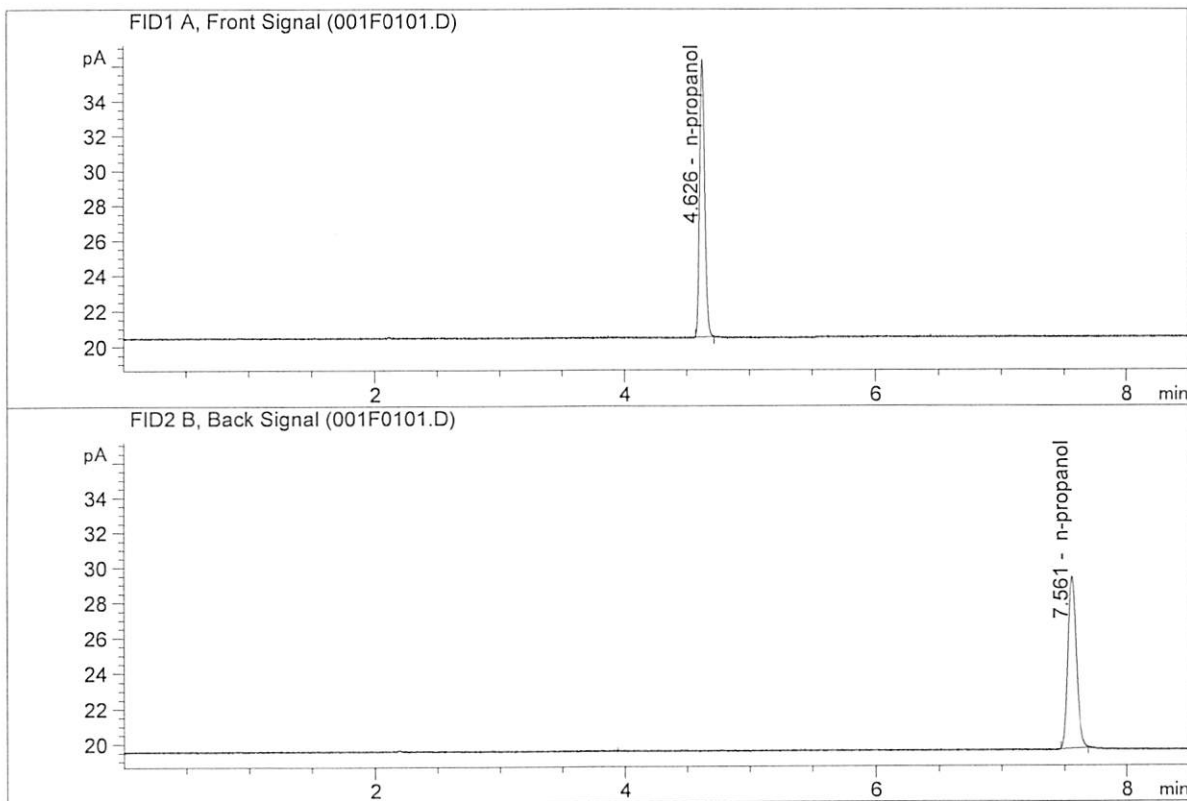


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	44.93129	1.0000	g/100cc
4.	n-Propanol	Column 2:	46.83789	1.0000	g/100cc

W

ISP Forensic Services Blood Alcohol Report

Sample Name : MIX VOL FN06041502
 Laboratory : Meridian
 Injection Date : Sep 12, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

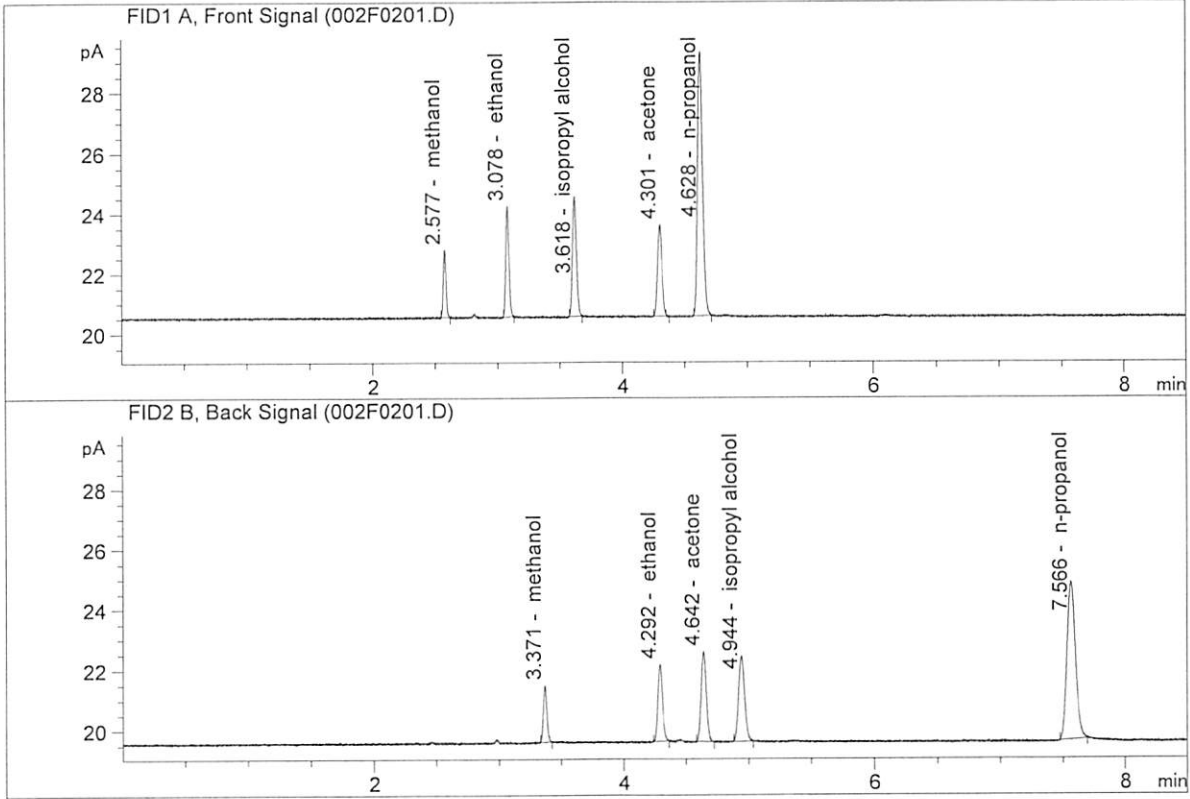

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	6.56198	0.1380	g/100cc
2.	Ethanol	Column 2:	6.72251	0.1386	g/100cc
3.	n-Propanol	Column 1:	24.64329	1.0000	g/100cc
4.	n-Propanol	Column 2:	25.06826	1.0000	g/100cc

[Handwritten signature]

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC1-1

Analysis Date(s): 12 Sep 2019

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.0792	0.0798	0.0006	0.0795	0.0793	
(g/100cc)	0.0790	0.0793	0.0003	0.0791		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: Alcohol.m
Hamilton Auto-Dilutor Serial Number: ML600HC11378

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%


Overall Mean (g/100cc)	Low	High	5% of Mean
0.079	0.075	0.083	0.004

	Reported Result	
	0.079	

Calibration and control data are stored centrally.


ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-1-A
 Laboratory : Meridian
 Injection Date : Sep 12, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

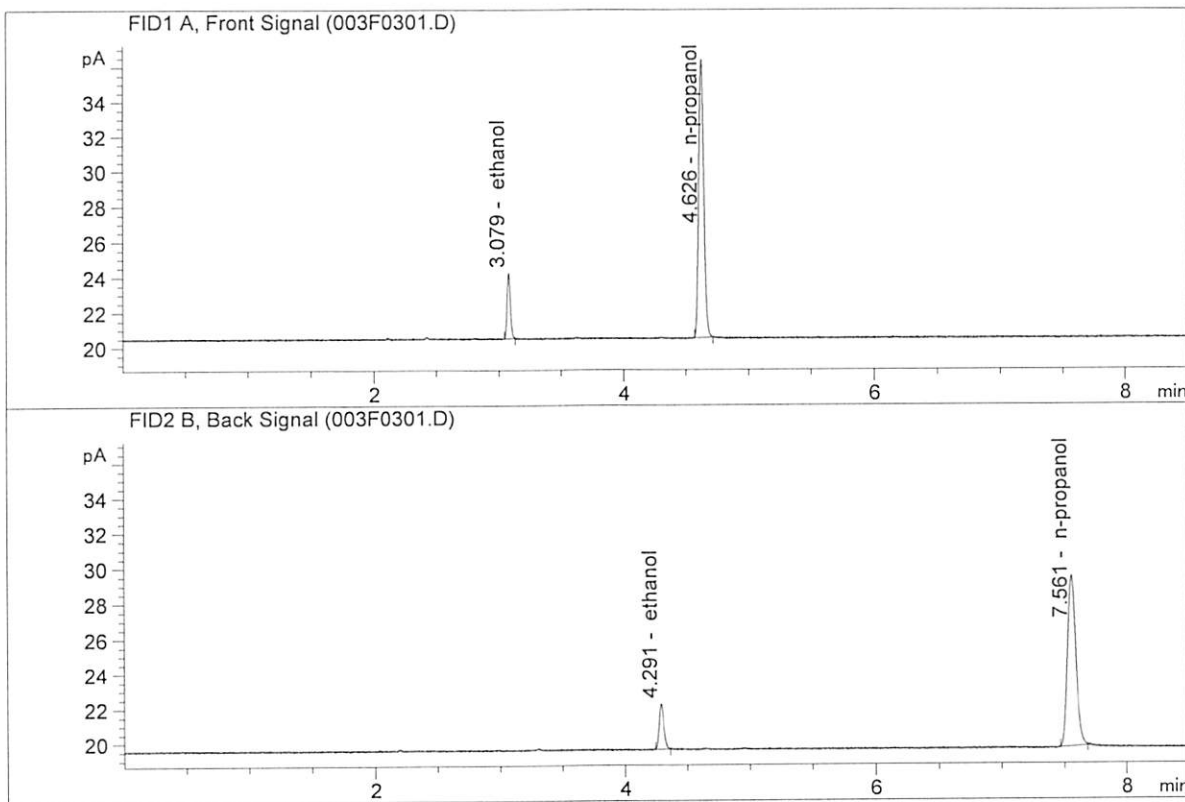


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	6.84064	0.0792	g/100cc
2.	Ethanol	Column 2:	7.01366	0.0798	g/100cc
3.	n-Propanol	Column 1:	45.10066	1.0000	g/100cc
4.	n-Propanol	Column 2:	46.64630	1.0000	g/100cc

Handwritten signature

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-1-B
 Laboratory : Meridian
 Injection Date : Sep 12, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

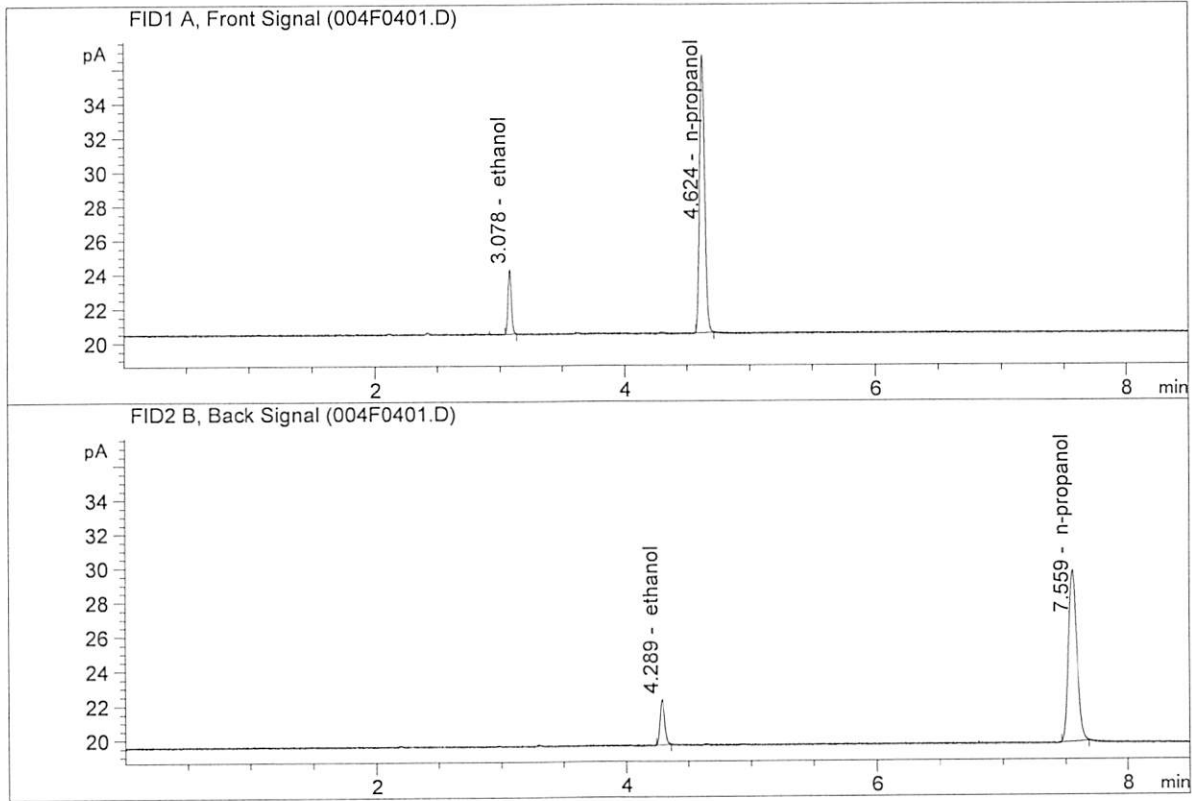

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	6.98191	0.0790	g/100cc
2.	Ethanol	Column 2:	7.13588	0.0793	g/100cc
3.	n-Propanol	Column 1:	46.14835	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.77390	1.0000	g/100cc

W

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: 0.08 FN04171701

Analysis Date(s): 12 Sep 2019

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.0801	0.0807	0.0006	0.0804	0.0806	
(g/100cc)	0.0807	0.0812	0.0005	0.0809		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: Alcohol.m
Hamilton Auto-Dilutor Serial Number: ML600HC11378

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.080	0.076	0.084	0.004


Reported Result	
0.080	

Calibration and control data are stored centrally.



ISP Forensic Services Blood Alcohol Report

Sample Name : 0.08 FN04171701-A
 Laboratory : Meridian
 Injection Date : Sep 12, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

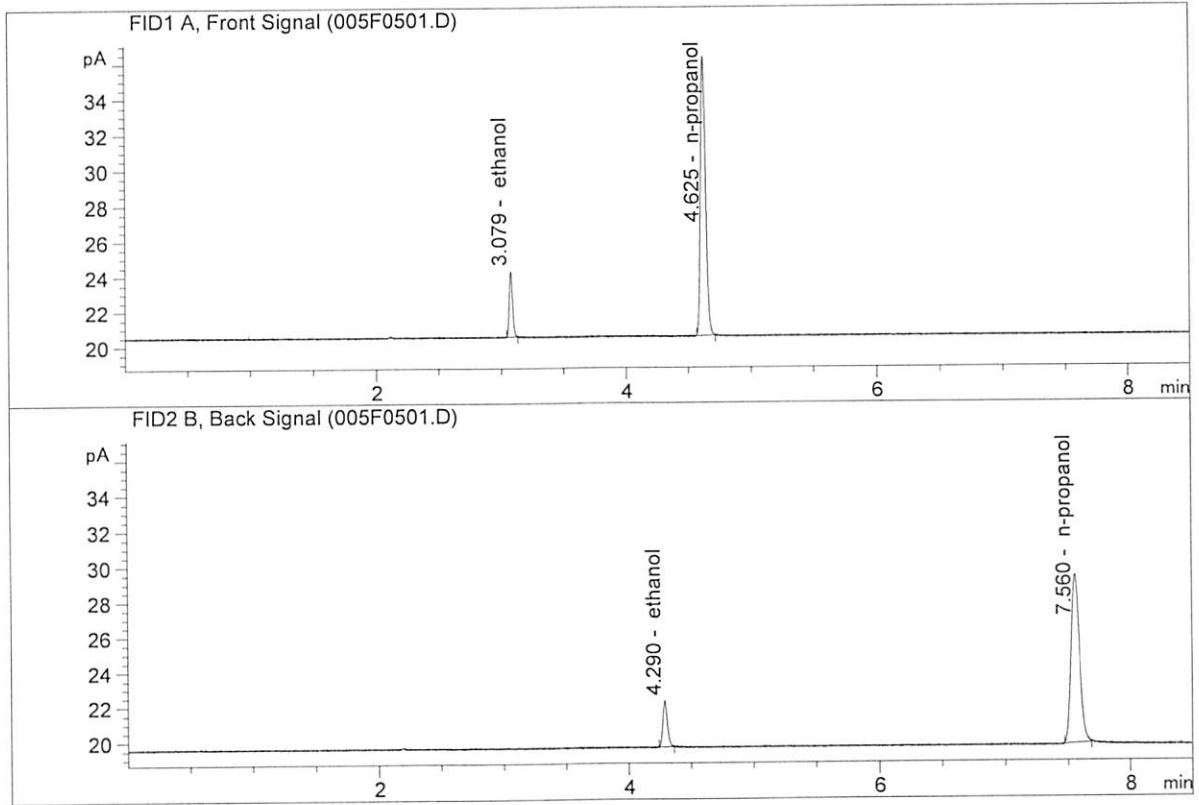


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	6.88378	0.0801	g/100cc
2.	Ethanol	Column 2:	7.05623	0.0807	g/100cc
3.	n-Propanol	Column 1:	44.85962	1.0000	g/100cc
4.	n-Propanol	Column 2:	46.36843	1.0000	g/100cc

W

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.08 FN04171701-B
 Laboratory : Meridian
 Injection Date : Sep 12, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

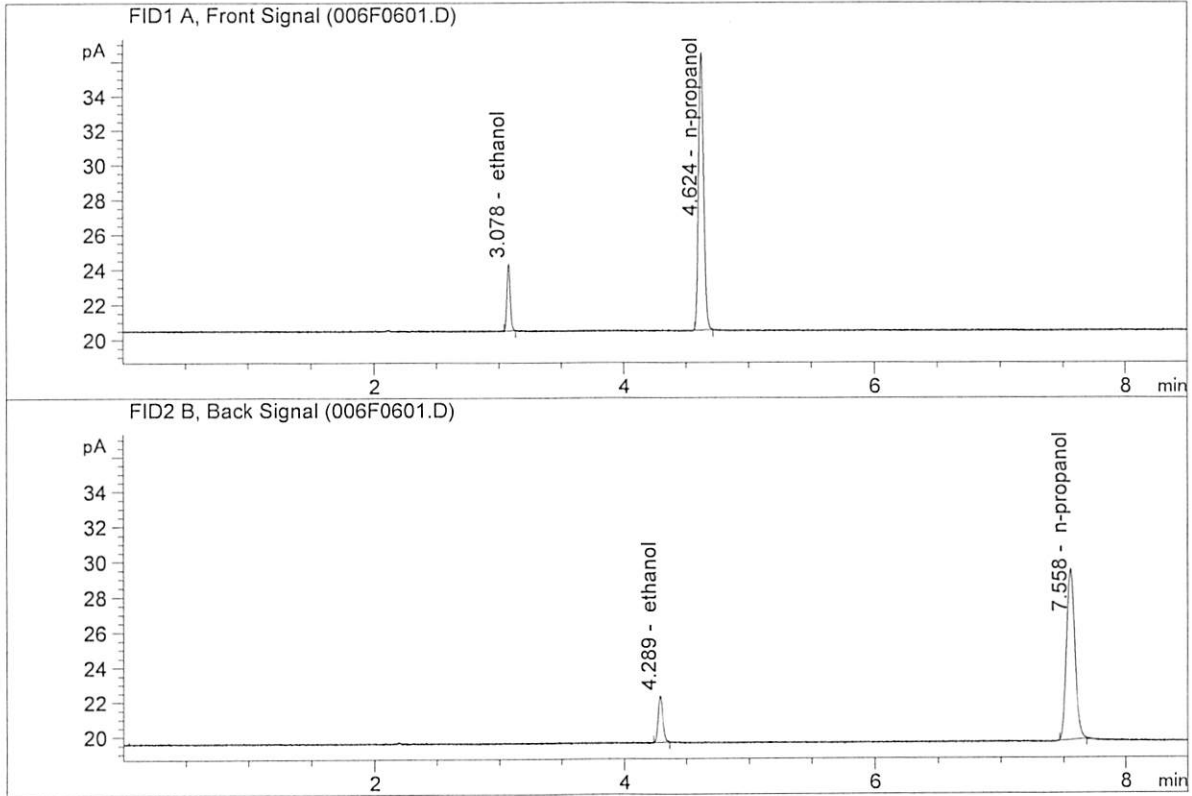

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.01876	0.0807	g/100cc
2.	Ethanol	Column 2:	7.16987	0.0812	g/100cc
3.	n-Propanol	Column 1:	45.37831	1.0000	g/100cc
4.	n-Propanol	Column 2:	46.84235	1.0000	g/100cc

[Handwritten signature]

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC2-1

Analysis Date(s): 12 Sep 2019

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.2018	0.2031	0.0013	0.2024	0.2038	
(g/100cc)	0.2052	0.2051	0.0001	0.2051		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: Alcohol.m
Hamilton Auto-Dilutor Serial Number: ML600HC11378

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%


Overall Mean (g/100cc)	Low	High	5% of Mean
0.203	0.192	0.214	0.011

	Reported Result	
	0.203	

Calibration and control data are stored centrally.


ISP Forensic Services Blood Alcohol Report

Sample Name : QC2-1-A
 Laboratory : Meridian
 Injection Date : Sep 12, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

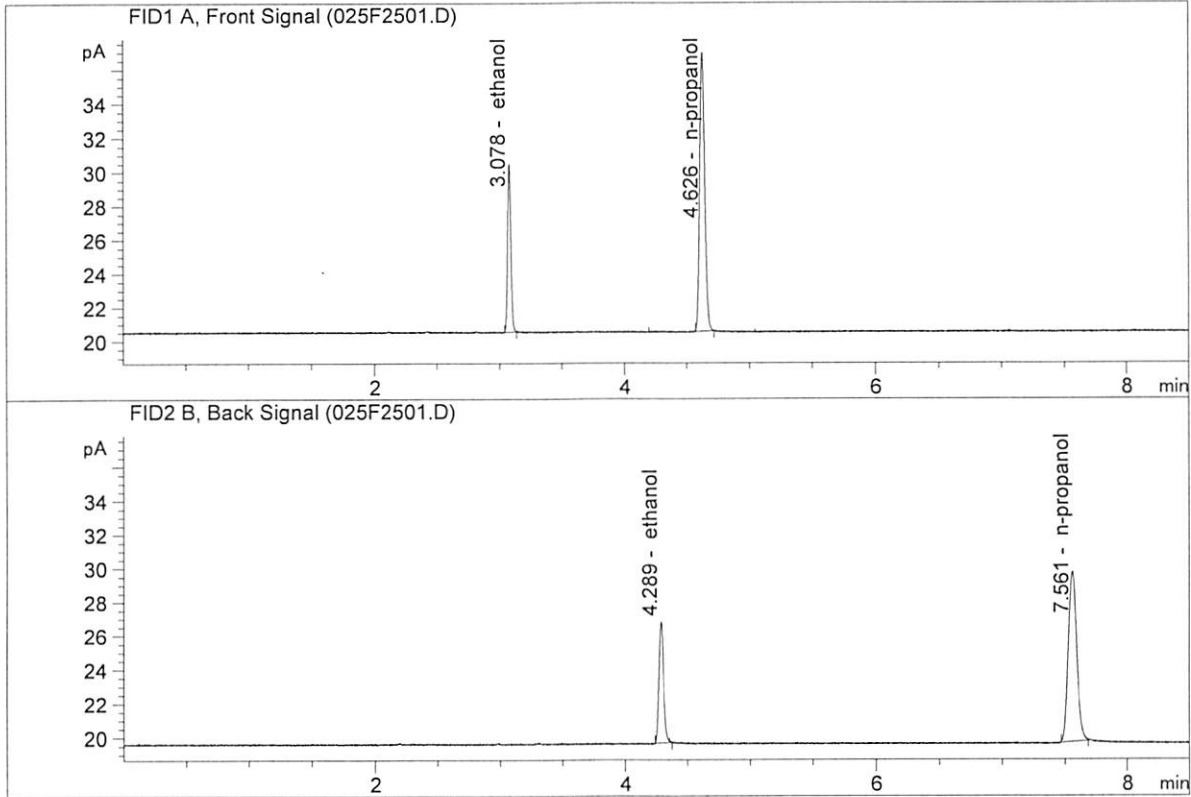


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	18.19839	0.2018	g/100cc
2.	Ethanol	Column 2:	19.13132	0.2031	g/100cc
3.	n-Propanol	Column 1:	46.60892	1.0000	g/100cc
4.	n-Propanol	Column 2:	48.13495	1.0000	g/100cc

W

ISP Forensic Services Blood Alcohol Report

Sample Name : QC2-1-B
 Laboratory : Meridian
 Injection Date : Sep 12, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

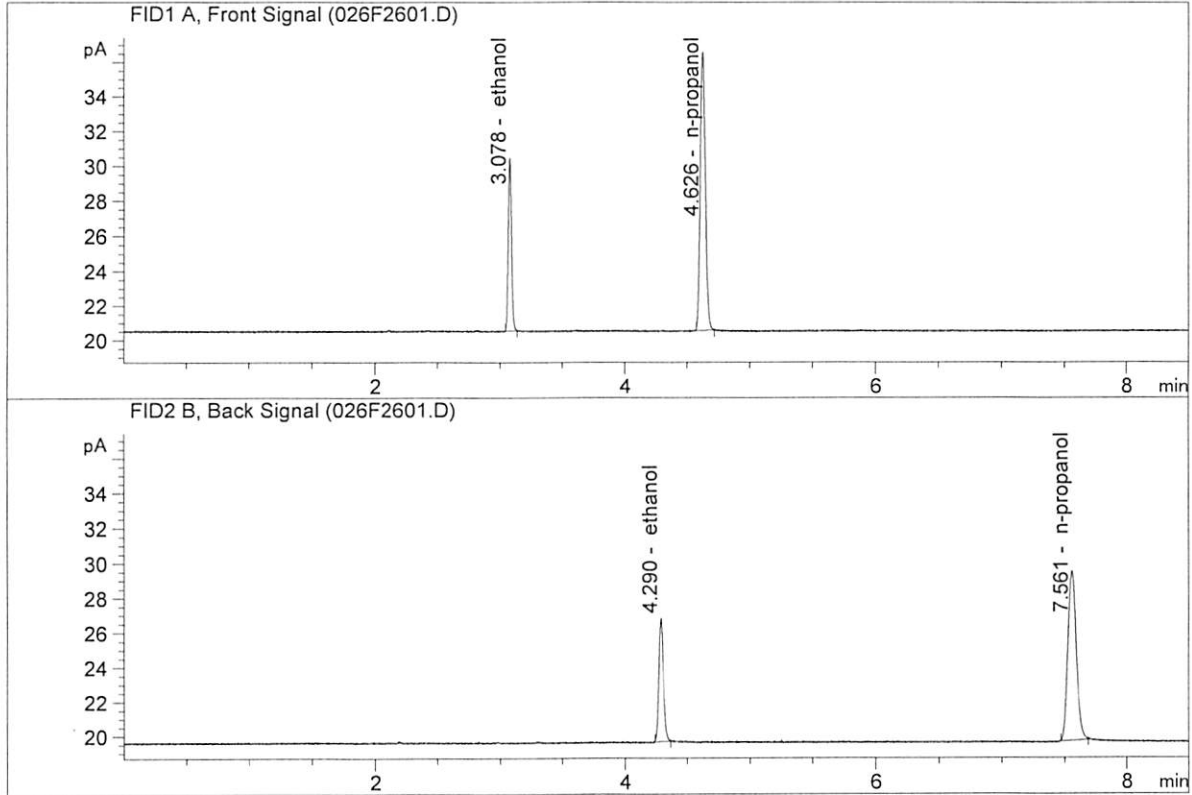

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	18.10089	0.2052	g/100cc
2.	Ethanol	Column 2:	18.92083	0.2051	g/100cc
3.	n-Propanol	Column 1:	45.58218	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.12168	1.0000	g/100cc

W

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC1-2

Analysis Date(s): 12 Sep 2019

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.0854	0.0864	0.0010	0.0859	0.0833	
(g/100cc)	0.0803	0.0811	0.0008	0.0807		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: Alcohol.m
Hamilton Auto-Dilutor Serial Number: ML600HC11378

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%


Overall Mean (g/100cc)	Low	High	5% of Mean
0.083	0.078	0.088	0.005

	Reported Result	
	0.083	

Calibration and control data are stored centrally.

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-2-A
 Laboratory : Meridian
 Injection Date : Sep 12, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

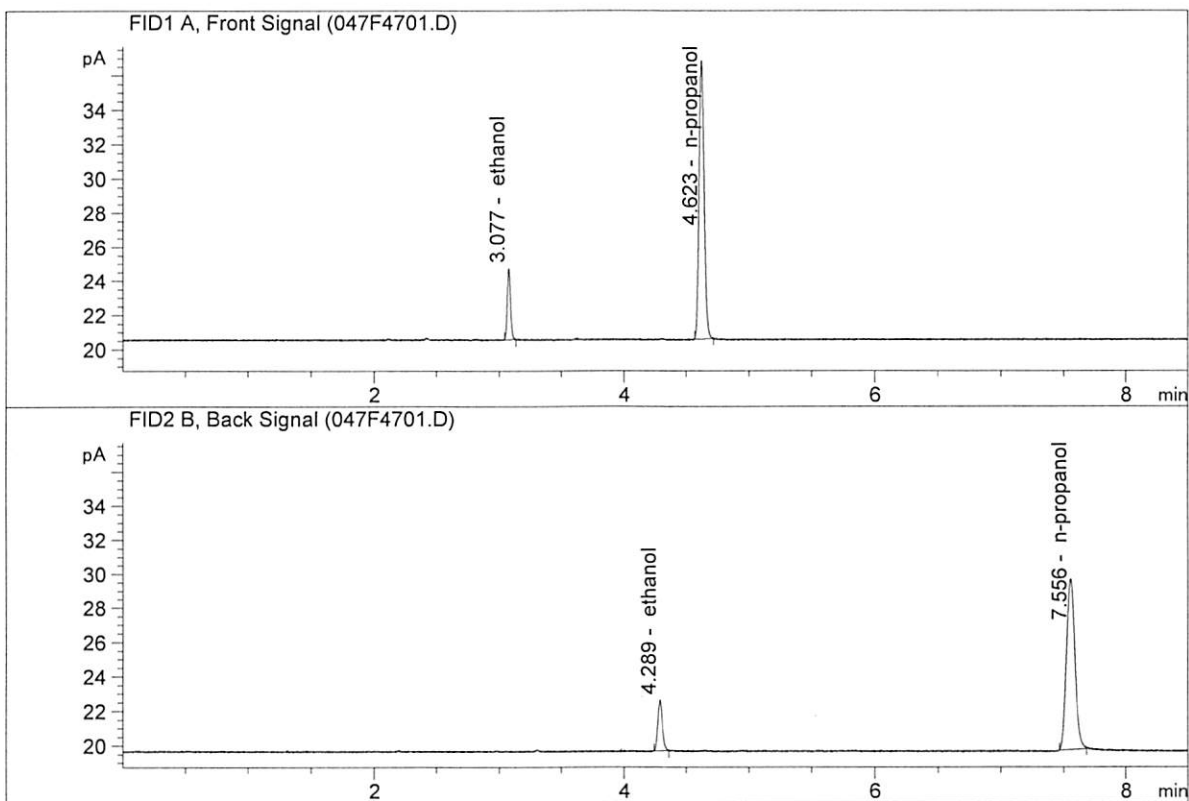


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.52562	0.0854	g/100cc
2.	Ethanol	Column 2:	7.74865	0.0864	g/100cc
3.	n-Propanol	Column 1:	45.92324	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.37063	1.0000	g/100cc

W

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-2-B
 Laboratory : Meridian
 Injection Date : Sep 12, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

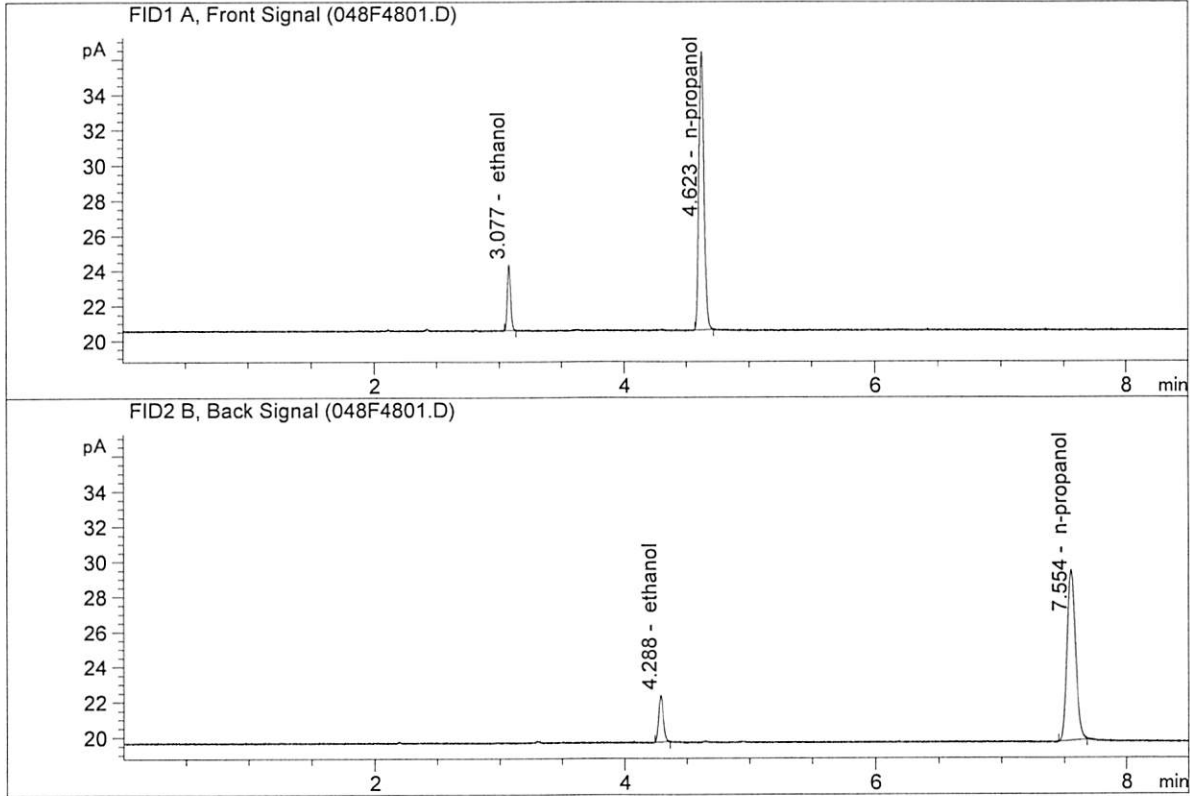

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	6.91544	0.0803	g/100cc
2.	Ethanol	Column 2:	7.11083	0.0811	g/100cc
3.	n-Propanol	Column 1:	44.95063	1.0000	g/100cc
4.	n-Propanol	Column 2:	46.51971	1.0000	g/100cc

W

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC2-2

Analysis Date(s): 12 Sep 2019

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Over-all Mean	
Sample Results	0.2035	0.2039	0.0004	0.2037	0.2026	
(g/100cc)	0.2013	0.2019	0.0006	0.2016		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument method is stored centrally.

Refer to Instrument Method: Alcohol.m
Hamilton Auto-Dilutor Serial Number: ML600HC11378

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.202	0.191	0.213	0.011

	Reported Result	
	0.202	

Calibration and control data are stored centrally.




Revision: 1

Issue Date: 01/04/2019

Issuing Authority: Quality Manager

ISP Forensic Services Blood Alcohol Report

Sample Name : QC2-2-A
 Laboratory : Meridian
 Injection Date : Sep 12, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

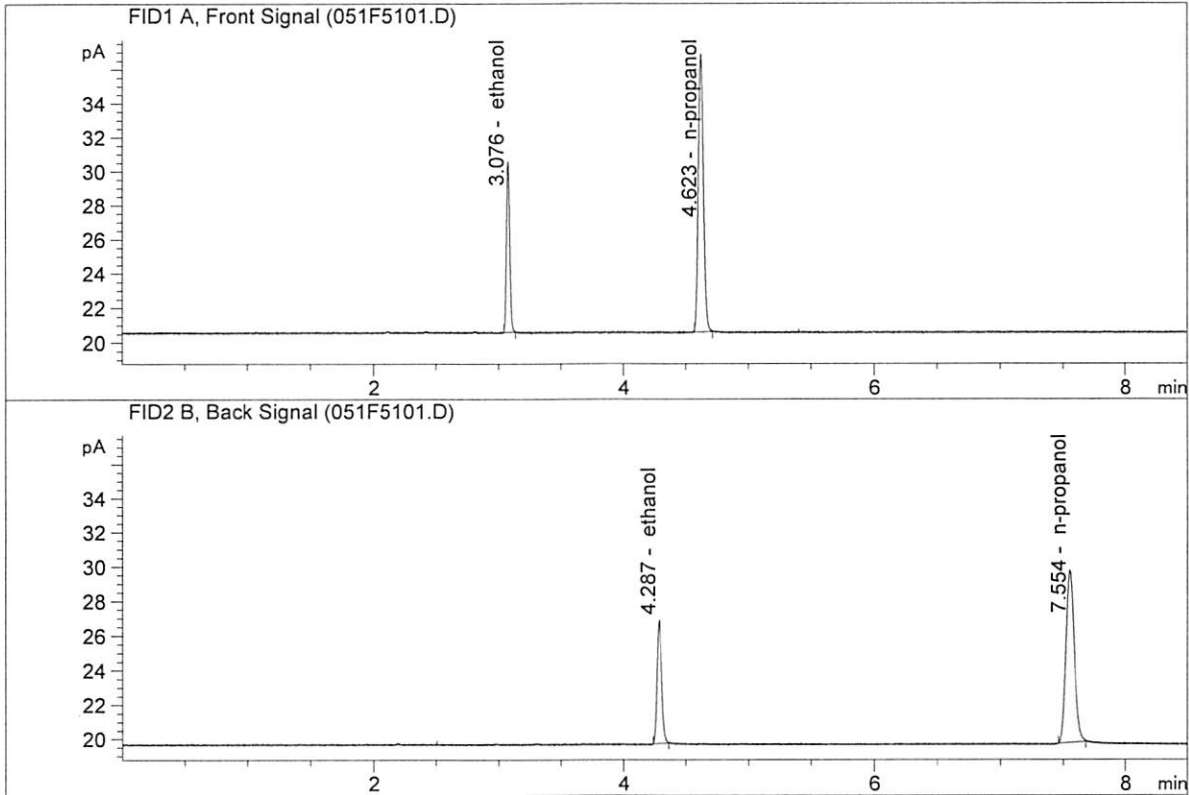


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	18.17113	0.2035	g/100cc
2.	Ethanol	Column 2:	19.01429	0.2039	g/100cc
3.	n-Propanol	Column 1:	46.14893	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.64783	1.0000	g/100cc

W

ISP Forensic Services Blood Alcohol Report

Sample Name : QC2-2-B
 Laboratory : Meridian
 Injection Date : Sep 12, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

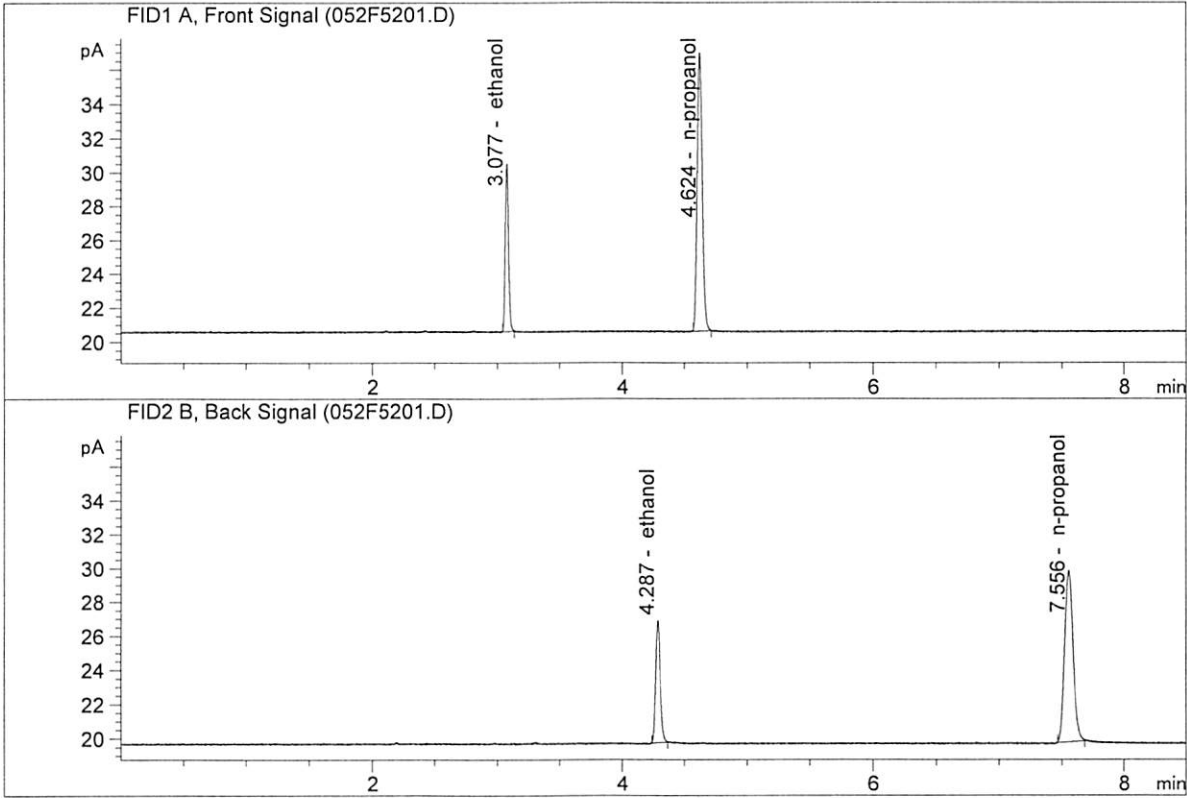


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	18.09827	0.2013	g/100cc
2.	Ethanol	Column 2:	18.96976	0.2019	g/100cc
3.	n-Propanol	Column 1:	46.46511	1.0000	g/100cc
4.	n-Propanol	Column 2:	48.00135	1.0000	g/100cc

W

ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STD BLK
 Laboratory : Meridian
 Injection Date : Sep 12, 2019
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

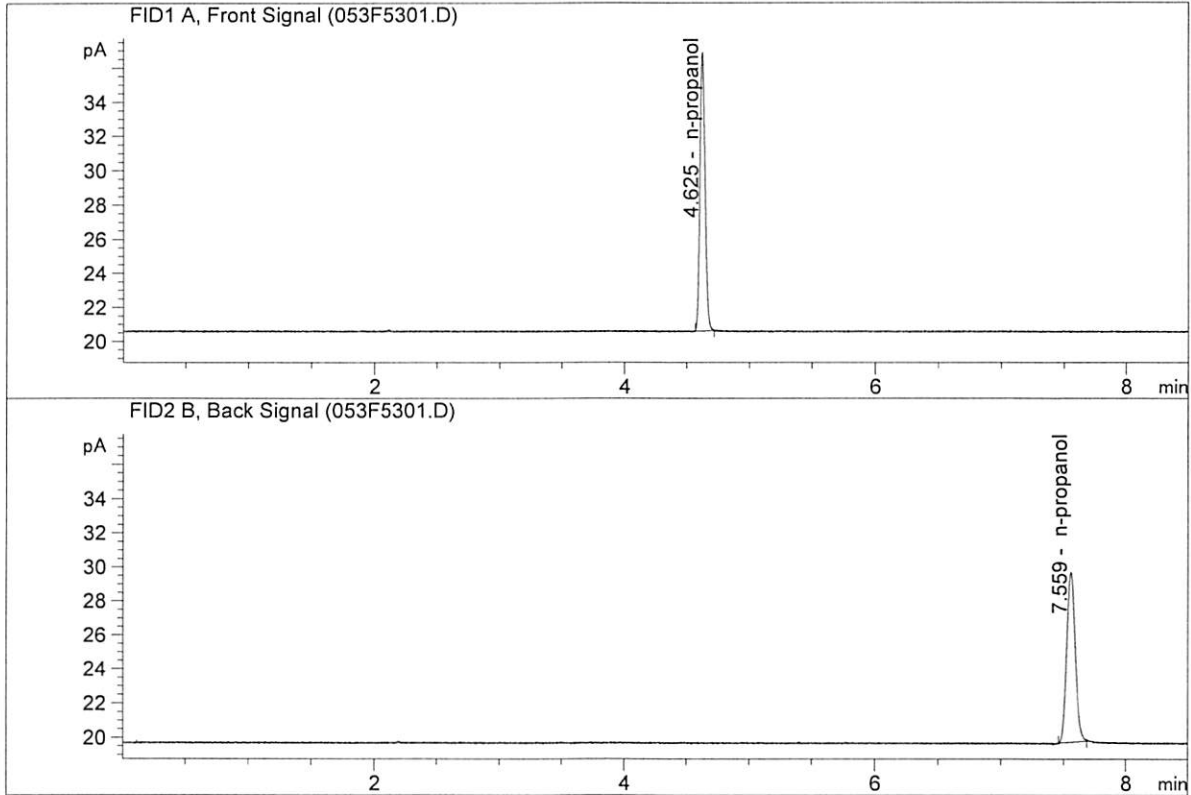

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	46.24262	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.90685	1.0000	g/100cc

W

S a m p l e S u m m a r y

Sequence table: C:\Chem32\1\Data\9-12-19_SAMPLES\09-12-19_SAMPLES 2019-09-12 11-56-53\09-12-19_SAMPLES.S
 Data directory path: C:\Chem32\1\Data\9-12-19_SAMPLES\09-12-19_SAMPLES 2019-09-12 11-56-53\
 Logbook: C:\Chem32\1\Data\9-12-19_SAMPLES\09-12-19_SAMPLES 2019-09-12 11-56-53\09-12-19_SAMPLES.LOG
 Sequence start: 9/12/2019 12:11:38 PM
 Sequence Operator: SYSTEM
 Operator: SYSTEM
 Method file name: C:\Chem32\1\Data\9-12-19_SAMPLES\09-12-19_SAMPLES 2019-09-12 11-56-53\ALCOHOL.M

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal # Cmp
1	1	1	INTERNAL STD BLK	-	1.0000	001F0101.D	2
2	2	1	MIX VOL FN060415	-	1.0000	002F0201.D	10
3	3	1	QC1-1-A	-	1.0000	003F0301.D	4
4	4	1	QC1-1-B	-	1.0000	004F0401.D	4
5	5	1	0.08 FN04171701-	-	1.0000	005F0501.D	4
6	6	1	0.08 FN04171701-	-	1.0000	006F0601.D	4
7	7	1	M2019-3926-1-A	-	1.0000	007F0701.D	4
8	8	1	M2019-3926-1-B	-	1.0000	008F0801.D	4
9	9	1	M2019-3927-1-A	-	1.0000	009F0901.D	2
10	10	1	M2019-3927-1-B	-	1.0000	010F1001.D	2
11	11	1	M2019-3934-1-A	-	1.0000	011F1101.D	4
12	12	1	M2019-3934-1-B	-	1.0000	012F1201.D	4
13	13	1	M2019-3935-1-A	-	1.0000	013F1301.D	4
14	14	1	M2019-3935-1-B	-	1.0000	014F1401.D	4
15	15	1	M2019-3940-1-A	-	1.0000	015F1501.D	4
16	16	1	M2019-3940-1-B	-	1.0000	016F1601.D	4
17	17	1	M2019-3954-1-A	-	1.0000	017F1701.D	4
18	18	1	M2019-3954-1-B	-	1.0000	018F1801.D	4
19	19	1	M2019-3955-1-A	-	1.0000	019F1901.D	4
20	20	1	M2019-3955-1-B	-	1.0000	020F2001.D	4
21	21	1	M2019-3962-1-A	-	1.0000	021F2101.D	4
22	22	1	M2019-3962-1-B	-	1.0000	022F2201.D	4
23	23	1	M2019-3972-2-A	-	1.0000	023F2301.D	2
24	24	1	M2019-3972-2-B	-	1.0000	024F2401.D	2
25	25	1	QC2-1-A	-	1.0000	025F2501.D	4
26	26	1	QC2-1-B	-	1.0000	026F2601.D	4
27	27	1	M2019-3974-1-A	-	1.0000	027F2701.D	4
28	28	1	M2019-3974-1-B	-	1.0000	028F2801.D	4
29	29	1	M2019-3975-1-A	-	1.0000	029F2901.D	4
30	30	1	M2019-3975-1-B	-	1.0000	030F3001.D	4
31	31	1	M2019-3976-1-A	-	1.0000	031F3101.D	4
32	32	1	M2019-3976-1-B	-	1.0000	032F3201.D	4
33	33	1	M2019-3977-1-A	-	1.0000	033F3301.D	4
34	34	1	M2019-3977-1-B	-	1.0000	034F3401.D	4
35	35	1	M2019-3991-1-A	-	1.0000	035F3501.D	2
36	36	1	M2019-3991-1-B	-	1.0000	036F3601.D	2
37	37	1	M2019-3991-2-A	-	1.0000	037F3701.D	2
38	38	1	M2019-3991-2-B	-	1.0000	038F3801.D	2
39	39	1	M2019-4017-1-A	-	1.0000	039F3901.D	4
40	40	1	M2019-4017-1-B	-	1.0000	040F4001.D	4
41	41	1	M2019-4065-1-A	-	1.0000	041F4101.D	4
42	42	1	M2019-4065-1-B	-	1.0000	042F4201.D	4
43	43	1	M2019-4066-1-A	-	1.0000	043F4301.D	4

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal # Cmp
44	44	1	M2019-4066-1-B	-	1.0000	044F4401.D	4
45	45	1	M2019-4110-1-A	-	1.0000	045F4501.D	4
46	46	1	M2019-4110-1-B	-	1.0000	046F4601.D	4
47	47	1	QC1-2-A	-	1.0000	047F4701.D	4
48	48	1	QC1-2-B	-	1.0000	048F4801.D	4
49	49	1	M2019-4112-1-A	-	1.0000	049F4901.D	4
50	50	1	M2019-4112-1-B	-	1.0000	050F5001.D	4
51	51	1	QC2-2-A	-	1.0000	051F5101.D	4
52	52	1	QC2-2-B	-	1.0000	052F5201.D	4
53	53	1	INTERNAL STD BLK	-	1.0000	053F5301.D	2

Method file name: C:\Chem32\1\Data\9-12-19_SAMPLES\09-12-19_SAMPLES 2019-09-12 11-56-53 \SHUTDOWN.M

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal # Cmp
54	54	1	EMPTY	-	1.0000	054F5401.D	0

W