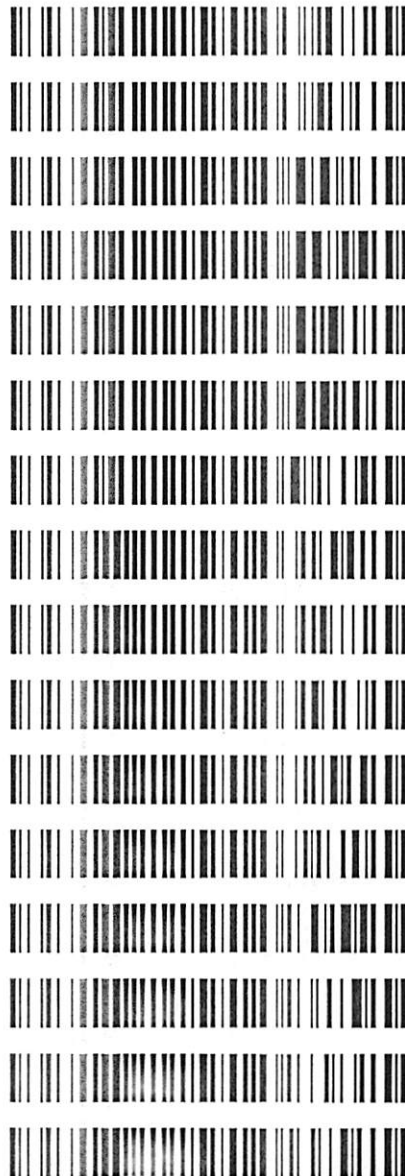


**Worklist: 4002**

| <u>LAB CASE</u> | <u>ITEM</u> | <u>ITEM TYPE</u> | <u>DESCRIPTION</u> |
|-----------------|-------------|------------------|--------------------|
| M2020-0554      | 1           | AALIQ            | Alcohol Analysis   |
| M2020-0555      | 1           | BCK              | Alcohol Analysis   |
| M2020-0591      | 1           | BCK              | Alcohol Analysis   |
| M2020-0592      | 2           | BCK              | Alcohol Analysis   |
| M2020-0593      | 1           | BCK              | Alcohol Analysis   |
| M2020-0594      | 1           | BCK              | Alcohol Analysis   |
| M2020-0645      | 1           | BCK              | Alcohol Analysis   |
| P2020-0392      | 1           | BCK              | Alcohol Analysis   |
| P2020-0393      | 1           | BCK              | Alcohol Analysis   |
| P2020-0395      | 1           | BCK              | Alcohol Analysis   |
| P2020-0404      | 1           | BCK              | Alcohol Analysis   |
| P2020-0407      | 1           | BCK              | Alcohol Analysis   |
| P2020-0422      | 1           | BCK              | Alcohol Analysis   |
| P2020-0423      | 1           | BCK              | Alcohol Analysis   |
| P2020-0430      | 1           | BCK              | Alcohol Analysis   |
| P2020-0447      | 1           | BCK              | Alcohol Analysis   |

**REVIEWED**

By Jeremy Johnston at 6:51 pm, Feb 17, 2020

**Quantitative Analysis for Ethanol & Qualitative Analysis for Other Volatiles**

*Analytical Method(s): 1.0*

**Device: Hamilton MICROLAB Liquid Processor/Dilutor Serial Number: ML600HC11378**

**Volatiles Quality Assurance Controls Run Date(s): 02/13/2020**

Calibration Date: 02/05/2020

| Control level                   | Expiration | Lot #   | Target Value    | Acceptable Range | Overall Results                             |
|---------------------------------|------------|---------|-----------------|------------------|---|
| Level 1                         | Jan-22     | 1801036 | 0.0812          | 0.0731-0.0893    | 0.0753 g/100cc<br>0.0767 g/100cc<br>g/100cc |
| Level 2                         | Mar-22     | 1803028 | 0.2035          | 0.1832-0.2238    | 0.1967 g/100cc<br>g/100cc                   |
| <b>Multi-Component mixture:</b> |            |         | <b>Lot #</b>    | FN06041502       | OK  |
| <b>Curve Fit:</b>               |            |         | <b>Column 1</b> | 1.0000           | <b>Column2</b>                              |
|                                 |            |         |                 |                  | 0.99994                                     |

**Ethanol Calibration Reference Material**


| Calibrator level | Target Value | Acceptable Range | Column 1 | Column 2 | Precision | Mean   |
|------------------|--------------|------------------|----------|----------|-----------|--------|
| 50               | 0.050        | 0.045 - 0.055    | 0.0504   | 0.0518   | 0.0014    | 0.0511 |
| 100              | 0.100        | 0.090 - 0.110    | 0.0997   | 0.1005   | 0.0008    | 0.1001 |
| 200              | 0.200        | 0.180 - 0.220    | 0.2001   | 0.1980   | 0.0021    | 0.199  |
| 300              | 0.300        | 0.270 - 0.330    | 0.2994   | 0.2980   | 0.0014    | 0.2987 |
| 400              | 0.400        | 0.360 - 0.440    |          |          |           |        |
| 500              | 0.500        | 0.450 - 0.550    | 0.5003   | 0.5017   | 0.0014    | 0.501  |

**Aqueous Controls**

| Control level | Target Value | Acceptable Range | Overall Results |
|---------------|--------------|------------------|-----------------|
| 80            | 0.080        | 0.076 - 0.084    | 0.078 g/100cc   |

ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STD BLK 1  
 Laboratory : Meridian  
 Injection Date : Feb 13, 2020  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

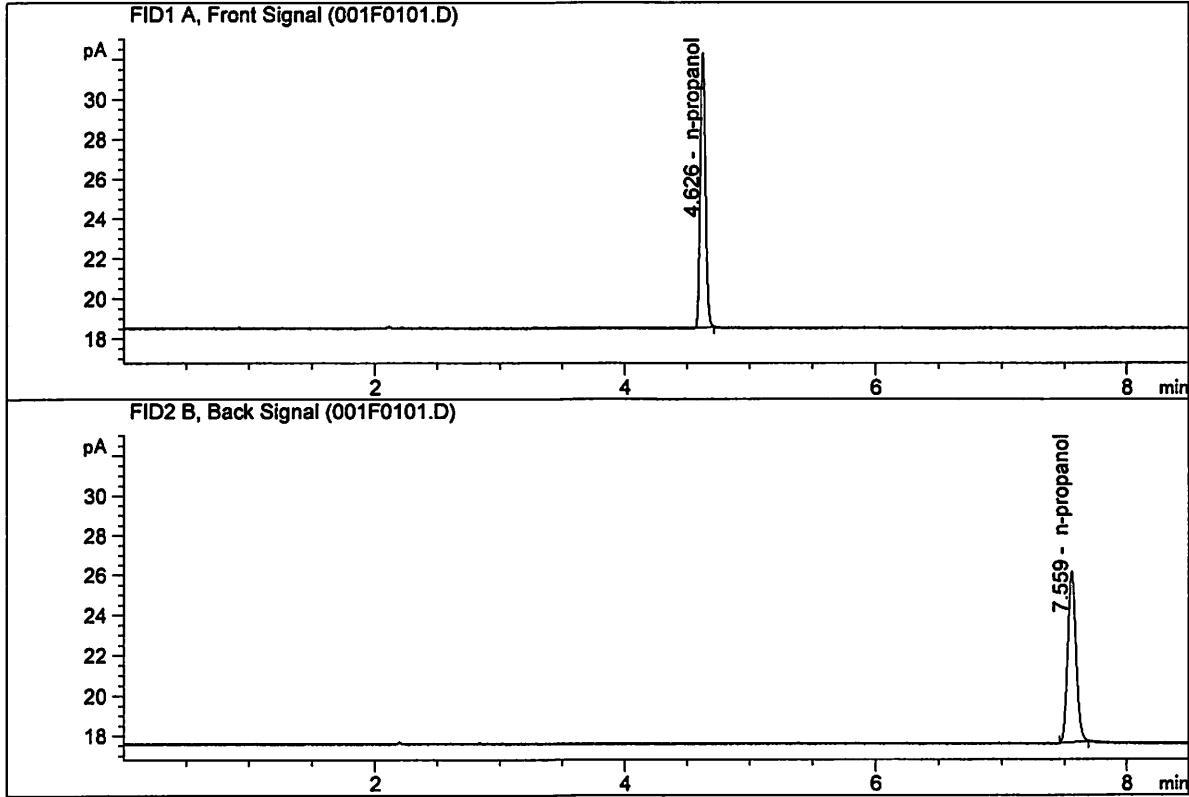


| #  | Compound   | Column    | Area     | Amount | Units   |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol    | Column 1: | 0.00000  | 0.0000 | g/100cc |
| 2. | Ethanol    | Column 2: | 0.00000  | 0.0000 | g/100cc |
| 3. | n-Propanol | Column 1: | 39.17781 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 40.89119 | 1.0000 | g/100cc |

*Handwritten signature*

ISP Forensic Services Blood Alcohol Report

Sample Name : MIX VOL FN06041502  
 Laboratory : Meridian  
 Injection Date : Feb 13, 2020  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

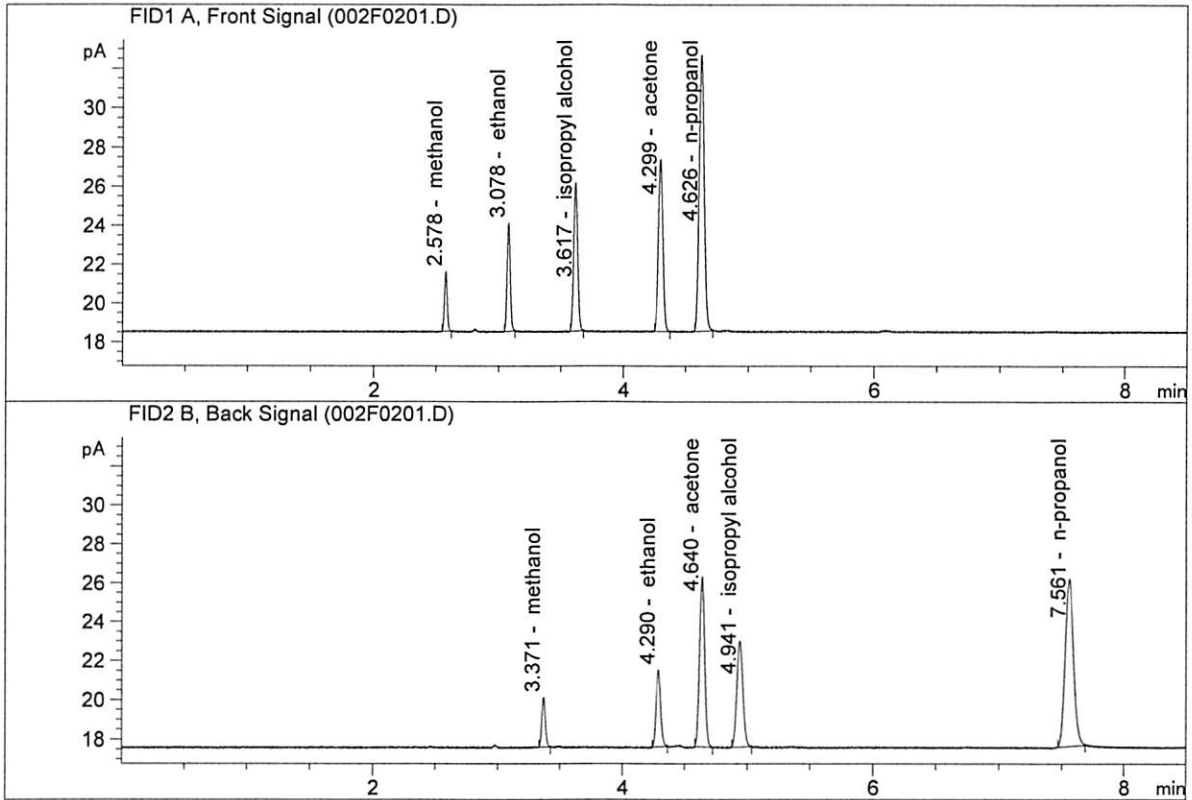

| #  | Compound   | Column    | Area     | Amount | Units   |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol    | Column 1: | 9.90730  | 0.1209 | g/100cc |
| 2. | Ethanol    | Column 2: | 10.30918 | 0.1214 | g/100cc |
| 3. | n-Propanol | Column 1: | 39.82067 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 41.06488 | 1.0000 | g/100cc |

*a*

## VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC1-1

Analysis Date(s): 13 Feb 2020

|                | Column 1<br>FID A | Column 2<br>FID B | Column Precision | Mean Value | Sample A-B<br>Difference | Over-all Mean |
|----------------|-------------------|-------------------|------------------|------------|--------------------------|---------------|
| Sample Results | 0.0743            | 0.0755            | 0.0012           | 0.0749     | 0.0008                   | 0.0753        |
| (g/100cc)      | 0.0750            | 0.0764            | 0.0014           | 0.0757     |                          |               |

### Analysis Method

Refer to Blood Alcohol Method #1

### Instrument Information

*Instrument information is stored centrally.*

Refer to Instrument Method: Alcohol.m

### Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

| Overall Mean (g/100cc) | Low   | High  | 5% of Mean |
|------------------------|-------|-------|------------|
| 0.075                  | 0.071 | 0.079 | 0.004      |


| Reported Result |  |
|-----------------|--|
| 0.075           |  |

*Calibration and control data are stored centrally.*


Revision: 2  
Issue Date: 12/23/2019

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-1-A  
 Laboratory : Meridian  
 Injection Date : Feb 13, 2020  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

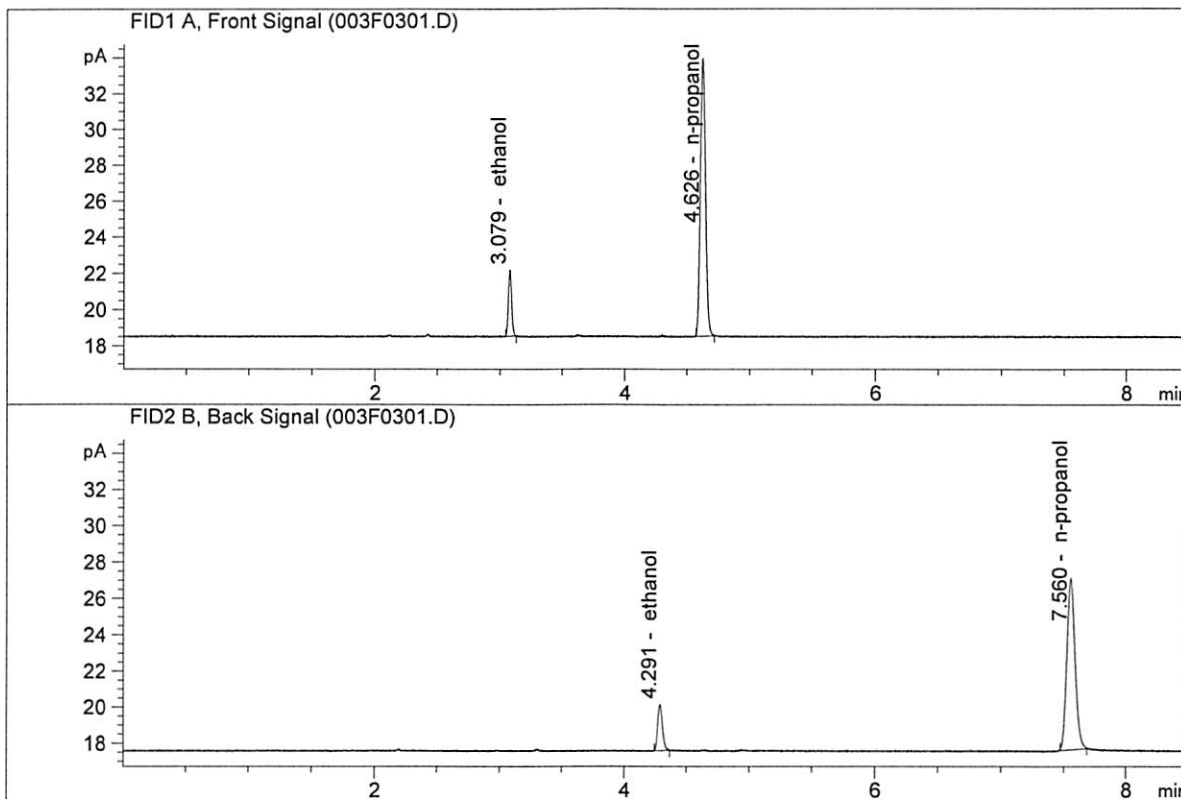


| #  | Compound   | Column    | Area     | Amount | Units   |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol    | Column 1: | 6.67959  | 0.0743 | g/100cc |
| 2. | Ethanol    | Column 2: | 6.88421  | 0.0755 | g/100cc |
| 3. | n-Propanol | Column 1: | 43.87432 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 45.28514 | 1.0000 | g/100cc |

*W*

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-1-B  
 Laboratory : Meridian  
 Injection Date : Feb 13, 2020  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

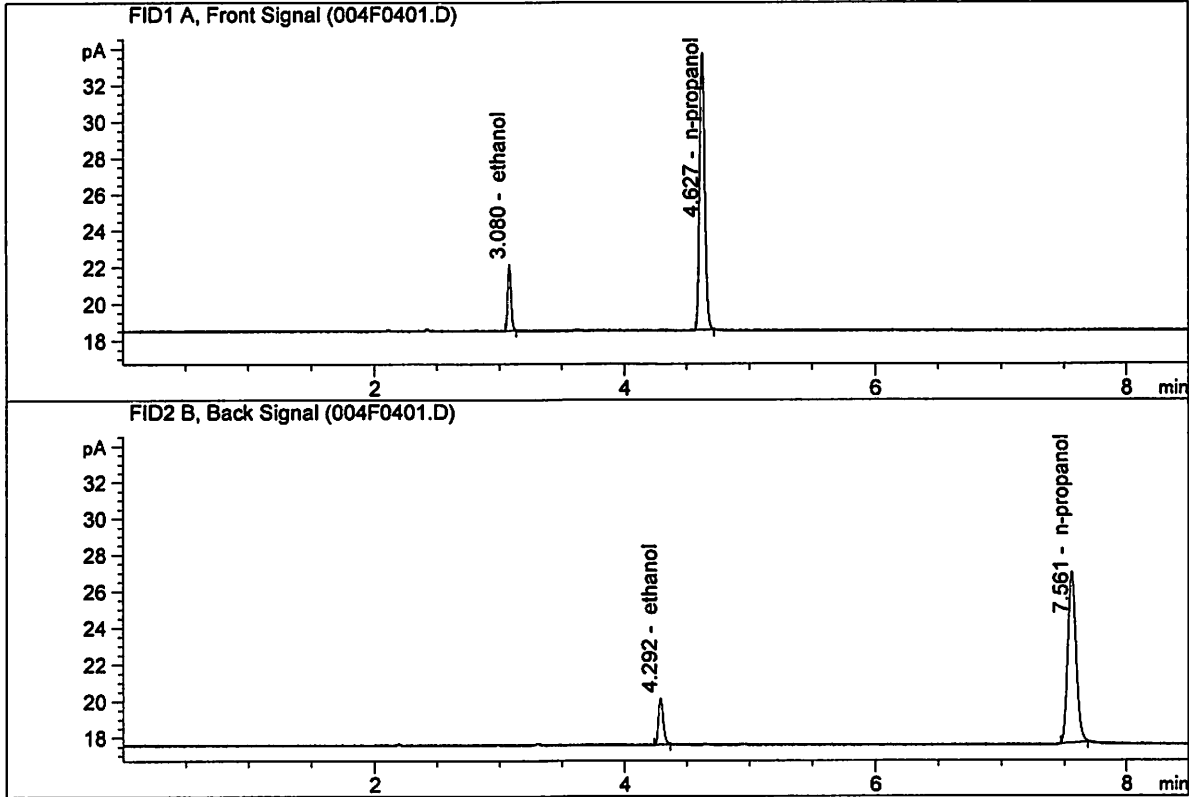

| #  | Compound   | Column    | Area     | Amount | Units   |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol    | Column 1: | 6.64807  | 0.0750 | g/100cc |
| 2. | Ethanol    | Column 2: | 6.88309  | 0.0764 | g/100cc |
| 3. | n-Propanol | Column 1: | 43.29032 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 44.69757 | 1.0000 | g/100cc |

*W*

## VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: 0.08 FN04171701

Analysis Date(s): 13 Feb 2020

|                | Column 1<br>FID A | Column 2<br>FID B | Column Precision | Mean Value | Sample A-B<br>Difference | Over-all Mean |
|----------------|-------------------|-------------------|------------------|------------|--------------------------|---------------|
| Sample Results | 0.0788            | 0.0798            | 0.0010           | 0.0793     | 0.0007                   | 0.0789        |
| (g/100cc)      | 0.0784            | 0.0788            | 0.0004           | 0.0786     |                          |               |

### Analysis Method

Refer to Blood Alcohol Method #1

### Instrument Information

*Instrument information is stored centrally.*

Refer to Instrument Method: Alcohol.m

### Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

| Overall Mean (g/100cc) | Low   | High  | 5% of Mean |
|------------------------|-------|-------|------------|
| 0.078                  | 0.074 | 0.082 | 0.004      |

|  | Reported Result |
|--|-----------------|
|  | 0.078           |


*Calibration and control data are stored centrally.*

W



ISP Forensic Services Blood Alcohol Report

Sample Name : 0.08 FN04171701-A  
 Laboratory : Meridian  
 Injection Date : Feb 13, 2020  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

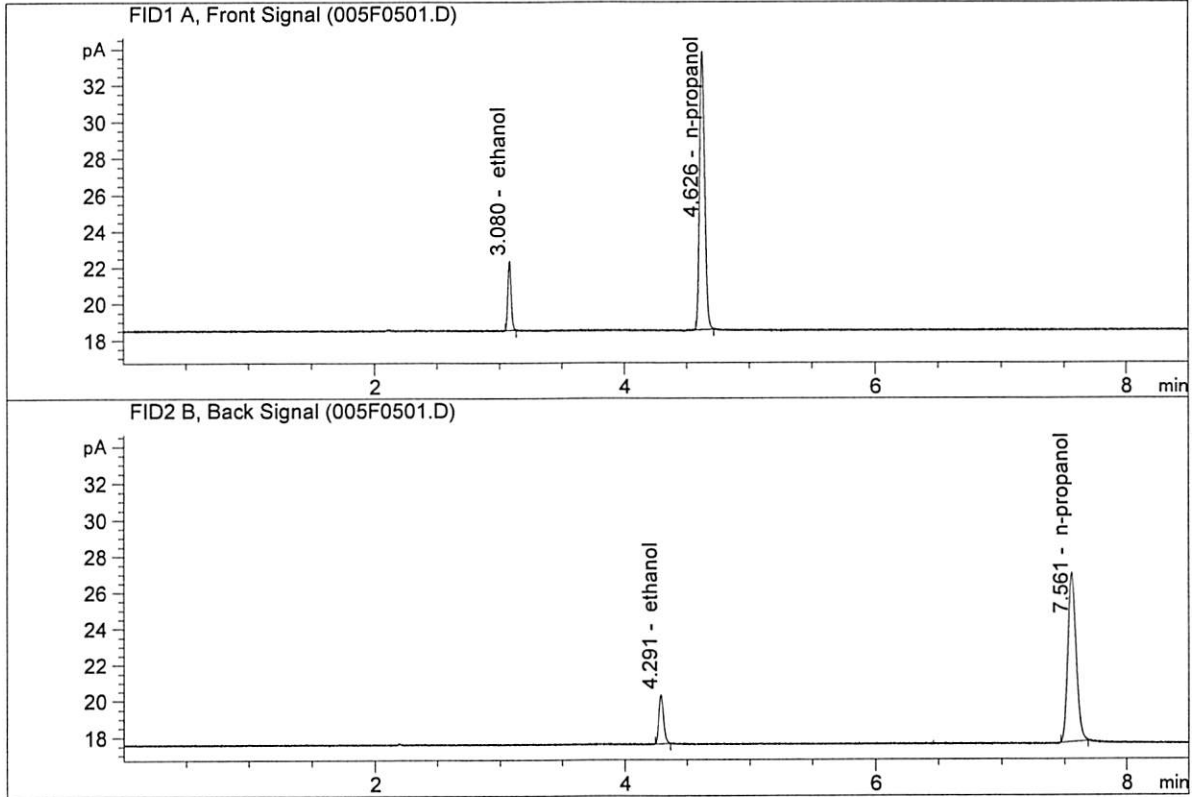


| #  | Compound   | Column    | Area     | Amount | Units   |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol    | Column 1: | 7.01431  | 0.0788 | g/100cc |
| 2. | Ethanol    | Column 2: | 7.22609  | 0.0798 | g/100cc |
| 3. | n-Propanol | Column 1: | 43.46008 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 44.81277 | 1.0000 | g/100cc |

*Handwritten signature*

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.08 FN04171701-B  
 Laboratory : Meridian  
 Injection Date : Feb 13, 2020  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

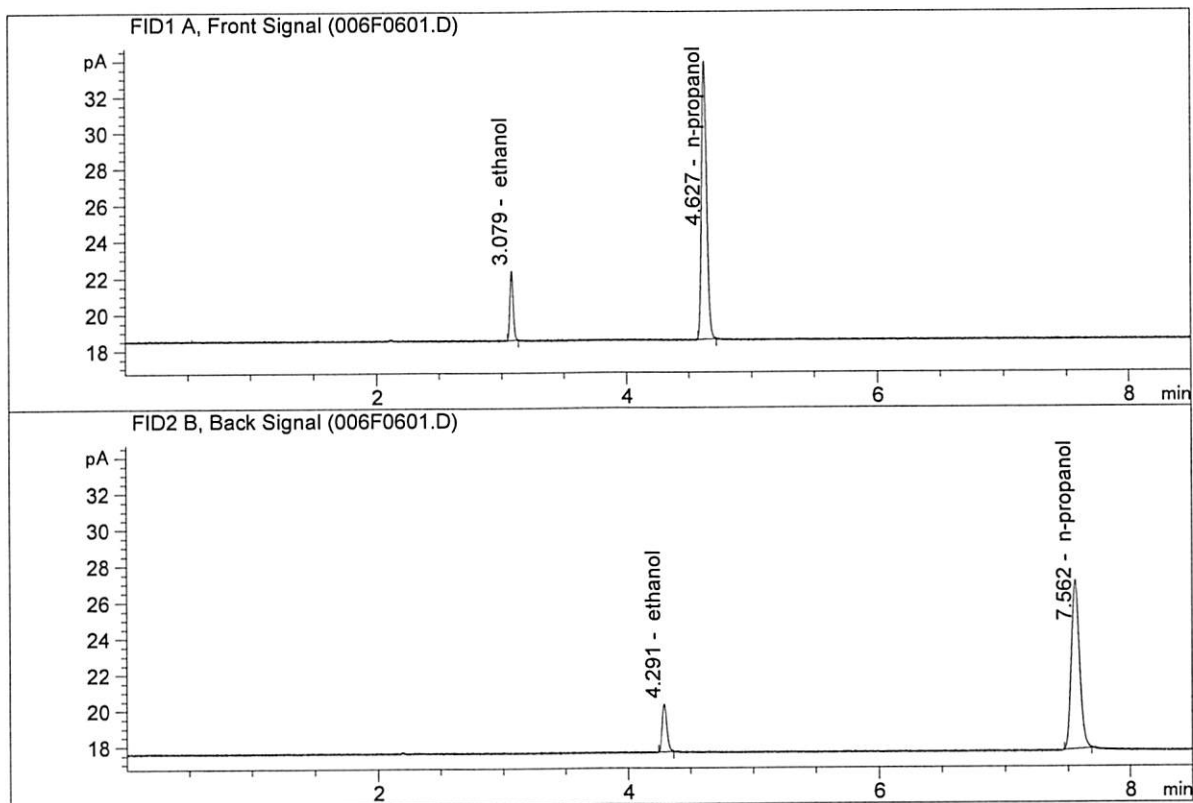

| #  | Compound   | Column    | Area     | Amount | Units   |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol    | Column 1: | 6.99540  | 0.0784 | g/100cc |
| 2. | Ethanol    | Column 2: | 7.12467  | 0.0788 | g/100cc |
| 3. | n-Propanol | Column 1: | 43.54966 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 44.78996 | 1.0000 | g/100cc |

*W*

## VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC2-1

Analysis Date(s): 13 Feb 2020

|                | Column 1<br>FID A | Column 2<br>FID B | Column Precision | Mean Value | Sample A-B<br>Difference | Over-all Mean |
|----------------|-------------------|-------------------|------------------|------------|--------------------------|---------------|
| Sample Results | 0.1962            | 0.1957            | 0.0005           | 0.1959     | 0.0016                   | 0.1967        |
| (g/100cc)      | 0.1972            | 0.1979            | 0.0007           | 0.1975     |                          |               |

### Analysis Method

Refer to Blood Alcohol Method #1

### Instrument Information

*Instrument information is stored centrally.*

Refer to Instrument Method: Alcohol.m

### Reporting of Results

Uncertainty of Measurement (UM%): 5.00%


| Overall Mean (g/100cc) | Low   | High  | 5% of Mean |
|------------------------|-------|-------|------------|
| 0.196                  | 0.186 | 0.206 | 0.010      |

| Reported Result |  |
|-----------------|--|
| 0.196           |  |

*Calibration and control data are stored centrally.*


ISP Forensic Services Blood Alcohol Report

Sample Name : QC2-1-A  
 Laboratory : Meridian  
 Injection Date : Feb 13, 2020  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

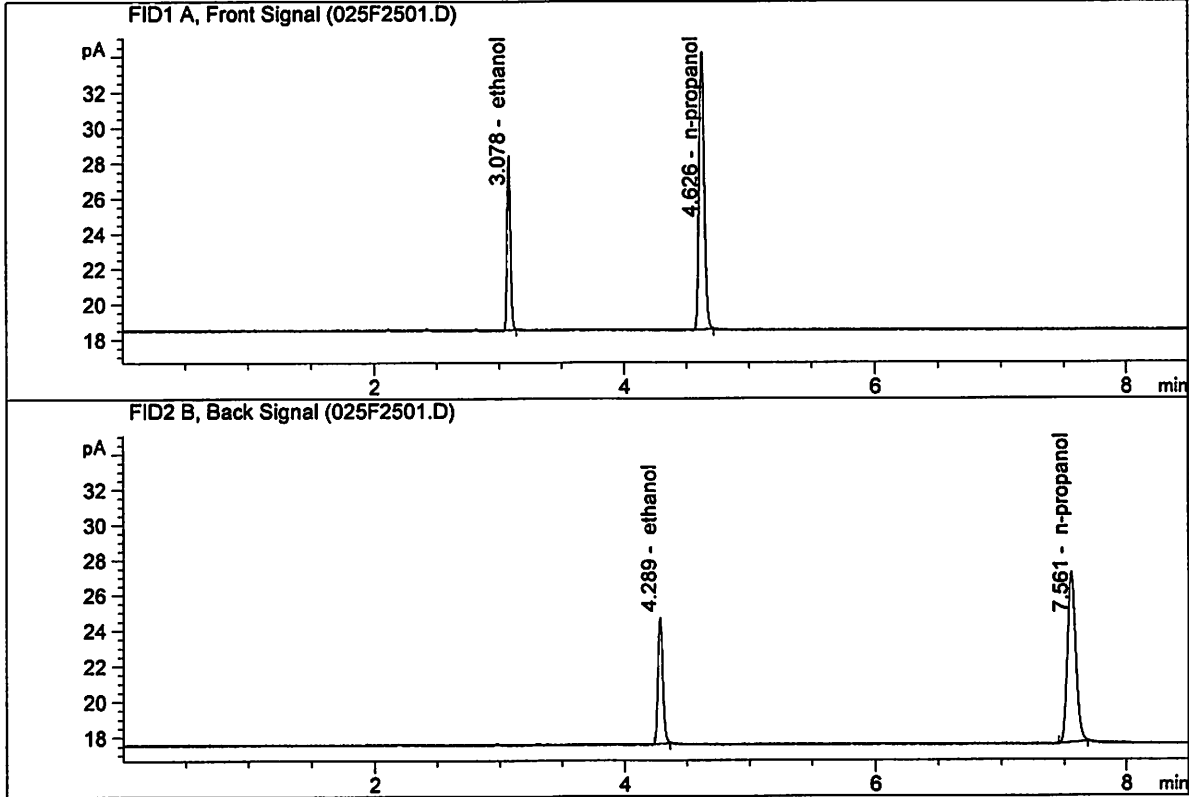


| #  | Compound   | Column    | Area     | Amount | Units   |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol    | Column 1: | 18.09829 | 0.1962 | g/100cc |
| 2. | Ethanol    | Column 2: | 18.84848 | 0.1957 | g/100cc |
| 3. | n-Propanol | Column 1: | 44.67163 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 45.82460 | 1.0000 | g/100cc |

W

ISP Forensic Services Blood Alcohol Report

Sample Name : QC2-1-B  
 Laboratory : Meridian  
 Injection Date : Feb 13, 2020  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

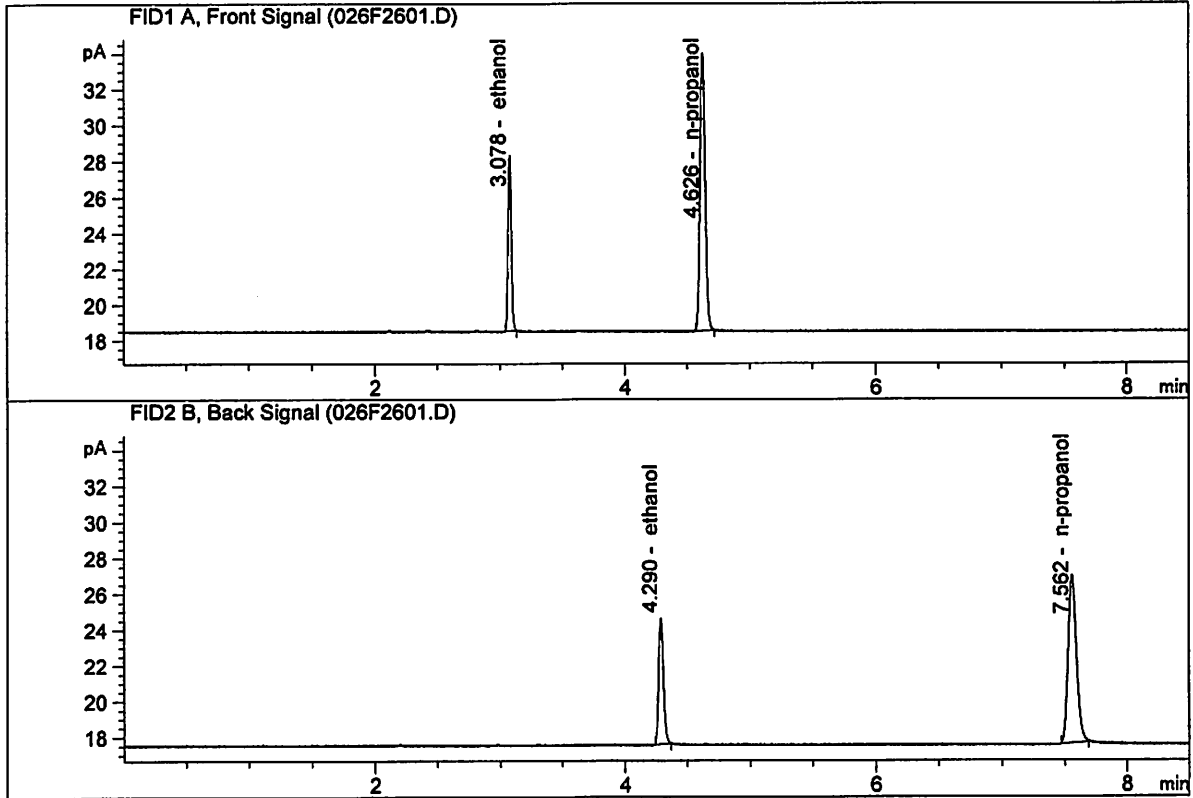

| #  | Compound   | Column    | Area     | Amount | Units   |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol    | Column 1: | 17.92922 | 0.1972 | g/100cc |
| 2. | Ethanol    | Column 2: | 18.72827 | 0.1979 | g/100cc |
| 3. | n-Propanol | Column 1: | 44.02166 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 45.02395 | 1.0000 | g/100cc |

*W*

## VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC1-2

Analysis Date(s): 13 Feb 2020

|                | Column 1<br>FID A | Column 2<br>FID B | Column Precision | Mean Value | Sample A-B<br>Difference | Over-all Mean |
|----------------|-------------------|-------------------|------------------|------------|--------------------------|---------------|
| Sample Results | 0.0757            | 0.0770            | 0.0013           | 0.0763     | 0.0008                   | 0.0767        |
| (g/100cc)      | 0.0764            | 0.0778            | 0.0014           | 0.0771     |                          |               |

### Analysis Method

Refer to Blood Alcohol Method #1

### Instrument Information

*Instrument information is stored centrally.*

Refer to Instrument Method: Alcohol.m

### Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

| Overall Mean (g/100cc) | Low   | High  | 5% of Mean |
|------------------------|-------|-------|------------|
| 0.076                  | 0.072 | 0.080 | 0.004      |

|  | Reported Result |  |
|--|-----------------|--|
|  | 0.076           |  |

*Calibration and control data are stored centrally.*

Revision: 2


Issue Date: 12/23/2019

Issuing Authority: Quality Manager

W

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-2-A  
 Laboratory : Meridian  
 Injection Date : Feb 13, 2020  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

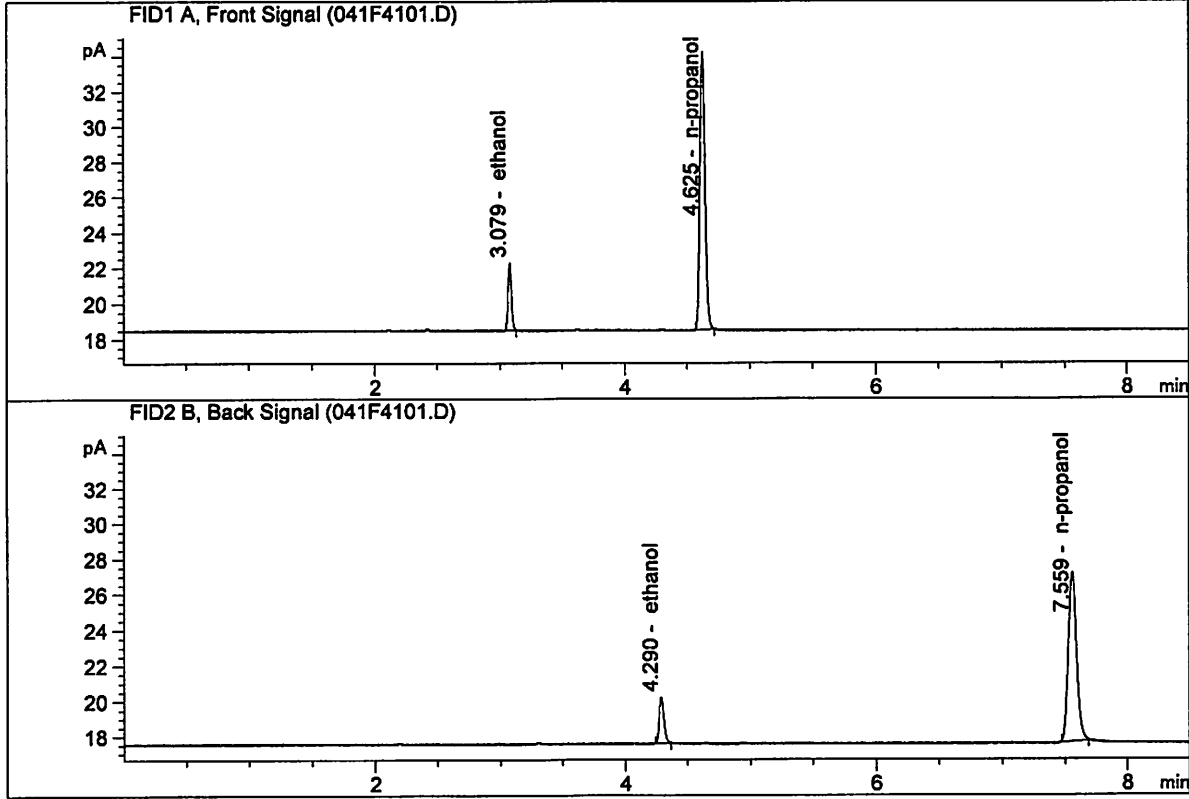


| #  | Compound   | Column    | Area     | Amount | Units   |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol    | Column 1: | 6.92930  | 0.0757 | g/100cc |
| 2. | Ethanol    | Column 2: | 7.09882  | 0.0770 | g/100cc |
| 3. | n-Propanol | Column 1: | 44.67289 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 45.71271 | 1.0000 | g/100cc |

*W*

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-2-B  
 Laboratory : Meridian  
 Injection Date : Feb 13, 2020  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

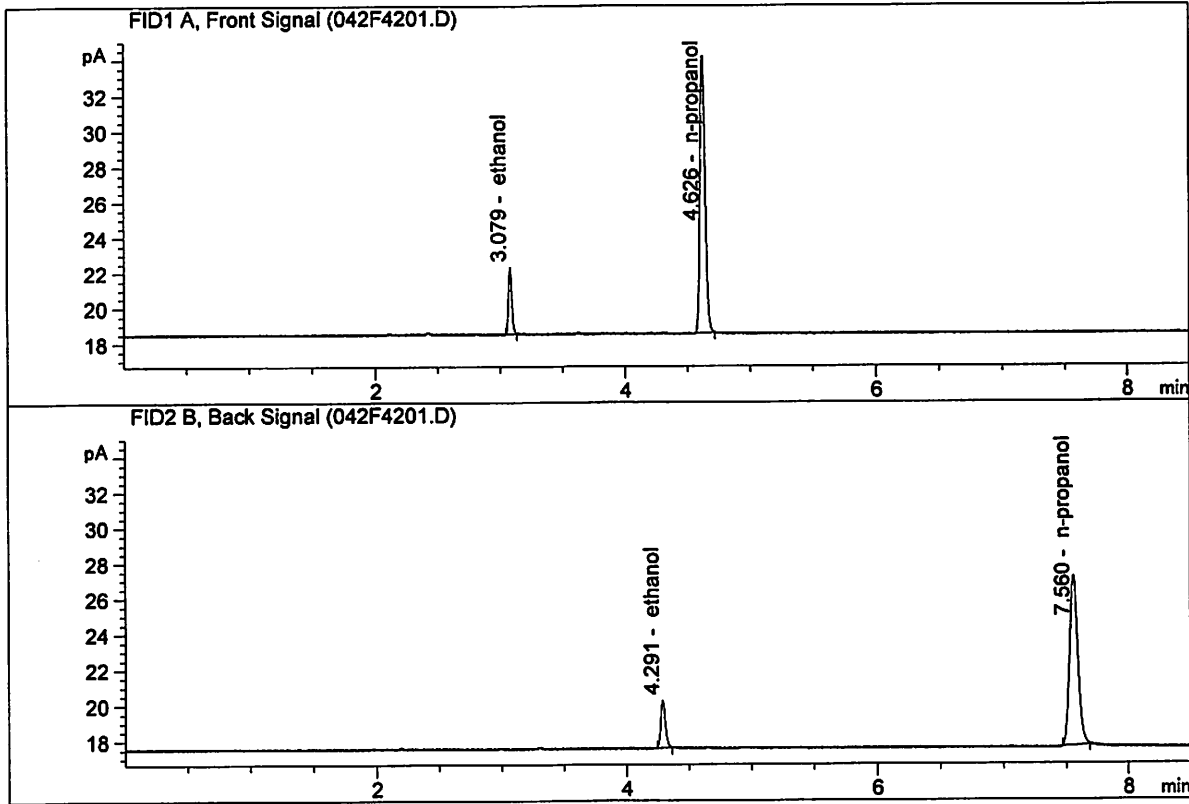


| #  | Compound   | Column    | Area     | Amount | Units   |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol    | Column 1: | 6.97191  | 0.0764 | g/100cc |
| 2. | Ethanol    | Column 2: | 7.14733  | 0.0778 | g/100cc |
| 3. | n-Propanol | Column 1: | 44.54357 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 45.56334 | 1.0000 | g/100cc |

*W*



ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STD BLK  
 Laboratory : Meridian  
 Injection Date : Feb 13, 2020  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

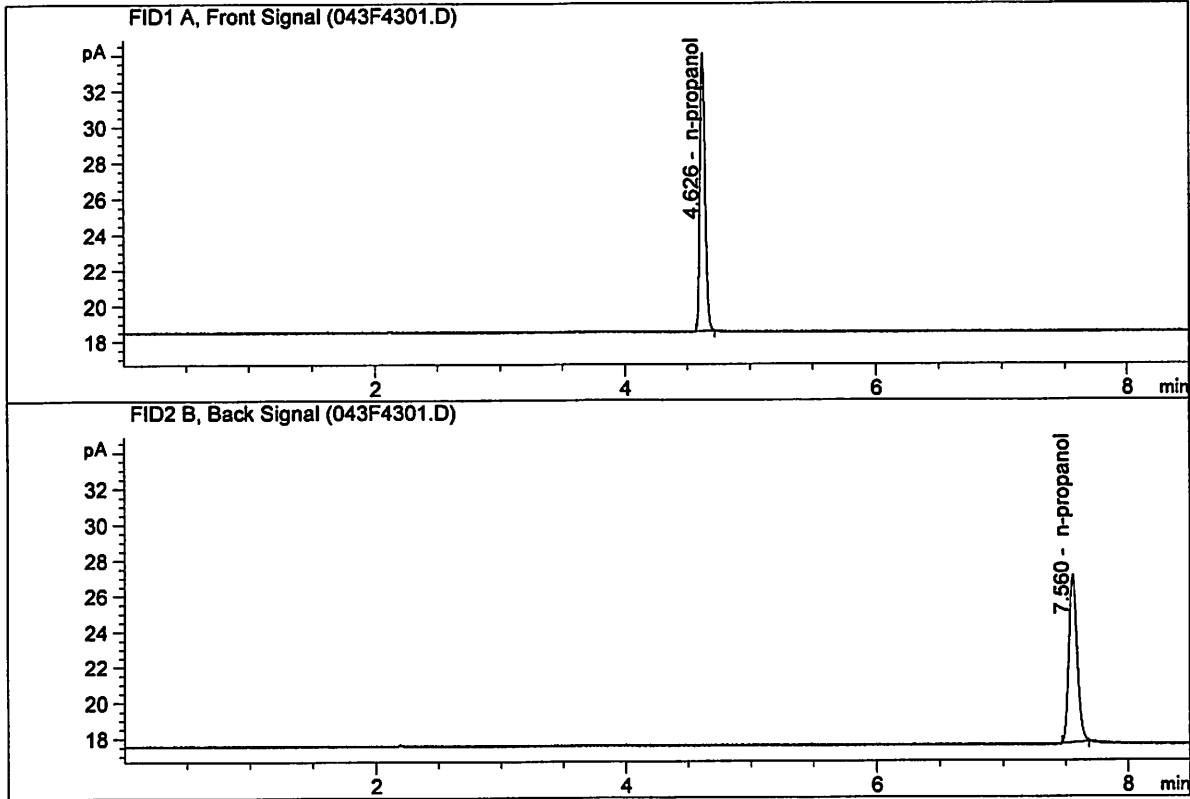

| #  | Compound   | Column    | Area     | Amount | Units   |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol    | Column 1: | 0.00000  | 0.0000 | g/100cc |
| 2. | Ethanol    | Column 2: | 0.00000  | 0.0000 | g/100cc |
| 3. | n-Propanol | Column 1: | 44.17923 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 45.07050 | 1.0000 | g/100cc |

*W*

## S a m p l e S u m m a r y

Sequence table: C:\Chem32\1\Data\02-13-20\_SAMPLES\02-13-20\_SAMPLES 2020-02-13 14-56-23\02-13-20\_SAMPLES.S  
 Data directory path: C:\Chem32\1\Data\02-13-20\_SAMPLES\02-13-20\_SAMPLES 2020-02-13 14-56-23\  
 Logbook: C:\Chem32\1\Data\02-13-20\_SAMPLES\02-13-20\_SAMPLES 2020-02-13 14-56-23\02-13-20\_SAMPLES.LOG  
 Sequence start: 2/13/2020 3:11:08 PM  
 Sequence Operator: SYSTEM  
 Operator: SYSTEM  
 Method file name: C:\Chem32\1\Data\02-13-20\_SAMPLES\02-13-20\_SAMPLES 2020-02-13 14-56-23\ALCOHOL.M

| Run # | Location # | Inj # | Sample Name      | Sample Amt [g/100cc] | Multip.* Dilution | File name  | Cal # | # Cmp |
|-------|------------|-------|------------------|----------------------|-------------------|------------|-------|-------|
| 1     | 1          | 1     | INTERNAL STD BLK | -                    | 1.0000            | 001F0101.D |       | 2     |
| 2     | 2          | 1     | MIX VOL FN060415 | -                    | 1.0000            | 002F0201.D |       | 10    |
| 3     | 3          | 1     | QC1-1-A          | -                    | 1.0000            | 003F0301.D |       | 4     |
| 4     | 4          | 1     | QC1-1-B          | -                    | 1.0000            | 004F0401.D |       | 4     |
| 5     | 5          | 1     | 0.08 FN04171701- | -                    | 1.0000            | 005F0501.D |       | 4     |
| 6     | 6          | 1     | 0.08 FN04171701- | -                    | 1.0000            | 006F0601.D |       | 4     |
| 7     | 7          | 1     | M2020-0554-1-A   | -                    | 1.0000            | 007F0701.D |       | 4     |
| 8     | 8          | 1     | M2020-0554-1-B   | -                    | 1.0000            | 008F0801.D |       | 4     |
| 9     | 9          | 1     | M2020-0555-1-A   | -                    | 1.0000            | 009F0901.D |       | 4     |
| 10    | 10         | 1     | M2020-0555-1-B   | -                    | 1.0000            | 010F1001.D |       | 4     |
| 11    | 11         | 1     | M2020-0591-1-A   | -                    | 1.0000            | 011F1101.D |       | 2     |
| 12    | 12         | 1     | M2020-0591-1-B   | -                    | 1.0000            | 012F1201.D |       | 2     |
| 13    | 13         | 1     | M2020-0592-2-A   | -                    | 1.0000            | 013F1301.D |       | 2     |
| 14    | 14         | 1     | M2020-0592-2-B   | -                    | 1.0000            | 014F1401.D |       | 2     |
| 15    | 15         | 1     | M2020-0593-1-A   | -                    | 1.0000            | 015F1501.D |       | 4     |
| 16    | 16         | 1     | M2020-0593-1-B   | -                    | 1.0000            | 016F1601.D |       | 4     |
| 17    | 17         | 1     | M2020-0594-1-A   | -                    | 1.0000            | 017F1701.D |       | 4     |
| 18    | 18         | 1     | M2020-0594-1-B   | -                    | 1.0000            | 018F1801.D |       | 4     |
| 19    | 19         | 1     | M2020-0645-1-A   | -                    | 1.0000            | 019F1901.D |       | 2     |
| 20    | 20         | 1     | M2020-0645-1-B   | -                    | 1.0000            | 020F2001.D |       | 2     |
| 21    | 21         | 1     | P2020-0392-1-A   | -                    | 1.0000            | 021F2101.D |       | 4     |
| 22    | 22         | 1     | P2020-0392-1-B   | -                    | 1.0000            | 022F2201.D |       | 4     |
| 23    | 23         | 1     | P2020-0393-1-A   | -                    | 1.0000            | 023F2301.D |       | 2     |
| 24    | 24         | 1     | P2020-0393-1-B   | -                    | 1.0000            | 024F2401.D |       | 2     |
| 25    | 25         | 1     | QC2-1-A          | -                    | 1.0000            | 025F2501.D |       | 4     |
| 26    | 26         | 1     | QC2-1-B          | -                    | 1.0000            | 026F2601.D |       | 4     |
| 27    | 27         | 1     | P2020-0395-1-A   | -                    | 1.0000            | 027F2701.D |       | 4     |
| 28    | 28         | 1     | P2020-0395-1-B   | -                    | 1.0000            | 028F2801.D |       | 4     |
| 29    | 29         | 1     | P2020-0404-1-A   | -                    | 1.0000            | 029F2901.D |       | 6     |
| 30    | 30         | 1     | P2020-0404-1-B   | -                    | 1.0000            | 030F3001.D |       | 6     |
| 31    | 31         | 1     | P2020-0407-1-A   | -                    | 1.0000            | 031F3101.D |       | 4     |
| 32    | 32         | 1     | P2020-0407-1-B   | -                    | 1.0000            | 032F3201.D |       | 4     |
| 33    | 33         | 1     | P2020-0422-1-A   | -                    | 1.0000            | 033F3301.D |       | 5     |
| 34    | 34         | 1     | P2020-0422-1-B   | -                    | 1.0000            | 034F3401.D |       | 6     |
| 35    | 35         | 1     | P2020-0423-1-A   | -                    | 1.0000            | 035F3501.D |       | 4     |
| 36    | 36         | 1     | P2020-0423-1-B   | -                    | 1.0000            | 036F3601.D |       | 4     |
| 37    | 37         | 1     | P2020-0430-1-A   | -                    | 1.0000            | 037F3701.D |       | 4     |
| 38    | 38         | 1     | P2020-0430-1-B   | -                    | 1.0000            | 038F3801.D |       | 4     |
| 39    | 39         | 1     | P2020-0447-1-A   | -                    | 1.0000            | 039F3901.D |       | 4     |
| 40    | 40         | 1     | P2020-0447-1-B   | -                    | 1.0000            | 040F4001.D |       | 6     |
| 41    | 41         | 1     | QC1-2-A          | -                    | 1.0000            | 041F4101.D |       | 4     |
| 42    | 42         | 1     | QC1-2-B          | -                    | 1.0000            | 042F4201.D |       | 4     |
| 43    | 43         | 1     | INTERNAL STD BLK | -                    | 1.0000            | 043F4301.D |       | 2     |

Method file name: C:\Chem32\1\Data\02-13-20\_SAMPLES\02-13-20\_SAMPLES 2020-02-13 14-56-23  
\SHUTDOWN.M

| Run # | Location | Inj # | Sample Name | Sample Amt [g/100cc] | Multip.* Dilution | File name  | Cal # |
|-------|----------|-------|-------------|----------------------|-------------------|------------|-------|
| 44    | 44       | 1     | EMPTY       | -                    | 1.0000            | 044F4401.D | 0     |



=====  
Calibration Table  
=====

-----  
General Calibration Setting  
-----

Calib. Data Modified : Wednesday, February 05, 2020 9:40:43 AM  
Signals calculated separately : No

Rel. Reference Window : 0.000 %  
Abs. Reference Window : 0.100 min  
Rel. Non-ref. Window : 0.000 %  
Abs. Non-ref. Window : 0.100 min  
Uncalibrated Peaks : not reported  
Partial Calibration : Yes, identified peaks are recalibrated  
Correct All Ret. Times: No, only for identified peaks

Curve Type : Linear  
Origin : Ignored  
Weight : Equal

Recalibration Settings:  
Average Response : Average all calibrations  
Average Retention Time: Floating Average New 75%

Calibration Report Options :  
Printout of recalibrations within a sequence:  
    Calibration Table after Recalibration  
    Normal Report after Recalibration  
If the sequence is done with bracketing:  
    Results of first cycle (ending previous bracket)

Default Sample ISTD Information (if not set in sample table):

| ISTD # | ISTD Amount [g/100cc] | Name       |
|--------|-----------------------|------------|
| 1      | 1.00000               | n-propanol |
| 2      | 1.00000               | n-propanol |

-----  
Signal Details  
-----

Signal 1: FID1 A, Front Signal  
Signal 2: FID2 B, Back Signal  
-----

-----  
Overview Table  
-----

| RT    | Sig | Lvl | Amount<br>[g/100cc] | Area     | Rsp.Factor | Ref | ISTD # | Compound          |
|-------|-----|-----|---------------------|----------|------------|-----|--------|-------------------|
| 2.586 | 1   | 1   | 1.00000             | 3.69669  | 2.70512e-1 | No  | No 1   | methanol          |
| 2.809 | 1   | 1   | 1.00000             | 4.26100  | 2.34687e-1 | No  | No 2   | Acetaldehyde      |
| 2.977 | 2   | 1   | 1.00000             | 4.26100  | 2.34687e-1 | No  | No 2   | Acetaldehyde      |
| 3.075 | 1   | 1   | 5.00000e-2          | 4.52242  | 1.10560e-2 | No  | No 1   | ethanol           |
|       |     |     | 1.00000e-1          | 9.04952  | 1.10503e-2 |     |        |                   |
|       |     |     | 2.00000e-1          | 18.19493 | 1.09921e-2 |     |        |                   |
|       |     |     | 3.00000e-1          | 27.40895 | 1.09453e-2 |     |        |                   |
|       |     |     | 5.00000e-1          | 45.87756 | 1.08986e-2 |     |        |                   |
| 3.388 | 2   | 1   | 1.00000             | 4.26062  | 2.34707e-1 | No  | No 2   | methanol          |
| 3.628 | 1   | 1   | 1.00000             | 9.73055  | 1.02769e-1 | No  | No 1   | isopropyl alcohol |
| 4.285 | 2   | 1   | 5.00000e-2          | 4.62532  | 1.08101e-2 | No  | No 2   | ethanol           |
|       |     |     | 1.00000e-1          | 9.39700  | 1.06417e-2 |     |        |                   |
|       |     |     | 2.00000e-1          | 18.84535 | 1.06127e-2 |     |        |                   |
|       |     |     | 3.00000e-1          | 28.70562 | 1.04509e-2 |     |        |                   |
|       |     |     | 5.00000e-1          | 48.52429 | 1.03041e-2 |     |        |                   |
| 4.308 | 1   | 1   | 1.00000             | 6.49940  | 1.53860e-1 | No  | No 1   | acetone           |
| 4.620 | 1   | 1   | 1.00000             | 44.08209 | 2.26850e-2 | No  | Yes 1  | n-propanol        |
|       |     |     | 1.00000             | 44.16013 | 2.26449e-2 |     |        |                   |
|       |     |     | 1.00000             | 44.01959 | 2.27172e-2 |     |        |                   |
|       |     |     | 1.00000             | 44.24614 | 2.26008e-2 |     |        |                   |
|       |     |     | 1.00000             | 44.25955 | 2.25940e-2 |     |        |                   |
| 4.661 | 2   | 1   | 1.00000             | 6.89301  | 1.45075e-1 | No  | No 2   | acetone           |
| 4.969 | 2   | 1   | 1.00000             | 10.70642 | 9.34019e-2 | No  | No 2   | isopropyl alcohol |
| 7.550 | 2   | 1   | 1.00000             | 45.86525 | 2.18030e-2 | No  | Yes 2  | n-propanol        |
|       |     |     | 1.00000             | 45.63153 | 2.19147e-2 |     |        |                   |
|       |     |     | 1.00000             | 45.28697 | 2.20814e-2 |     |        |                   |
|       |     |     | 1.00000             | 45.42099 | 2.20163e-2 |     |        |                   |
|       |     |     | 1.00000             | 45.29530 | 2.20773e-2 |     |        |                   |


Peak Sum Table

\*\*\*No Entries in table\*\*\*

1 Warnings or Errors :


Warning : Curve requires more calibration points., (methanol)

Calibration Curves

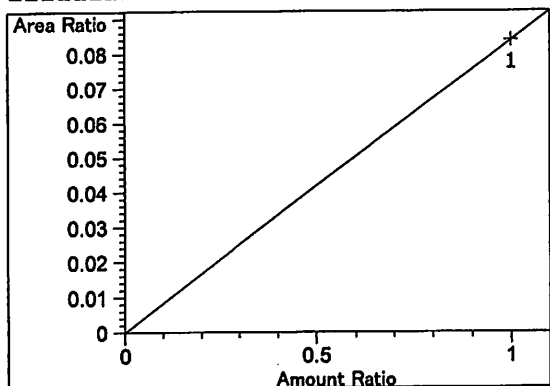


methanol at exp. RT: 2.586  
 FID1 A, Front Signal  
 Correlation: 1.00000  
 Residual Std. Dev.: 0.00000  
 Formula:  $y = mx + b$   
 m: 8.38593e-2  
 b: 0.00000  
 x: Amount Ratio  
 y: Area Ratio


N

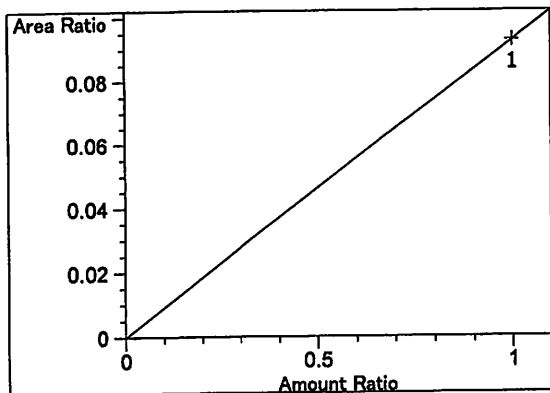


Acetaldehyde at exp. RT: 2.809  
 FID1 A, Front Signal  
 Correlation: 1.00000  
 Residual Std. Dev.: 0.00000  
 Formula:  $y = mx + b$   
 m: 9.29026e-2  
 b: 0.00000  
 x: Amount Ratio  
 y: Area Ratio

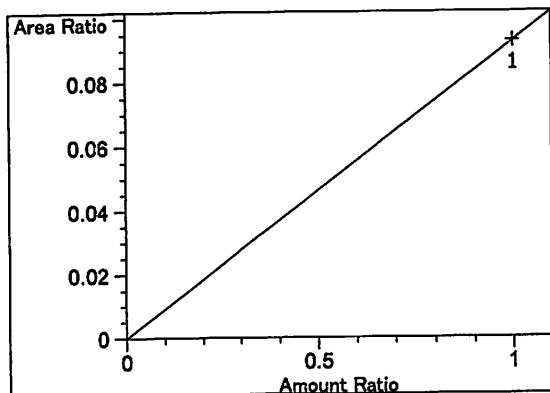

Acetaldehyde at exp. RT: 2.977  
 FID2 B, Back Signal  
 Correlation: 1.00000  
 Residual Std. Dev.: 0.00000  
 Formula:  $y = mx + b$   
 m: 9.29026e-2  
 b: 0.00000  
 x: Amount Ratio  
 y: Area Ratio

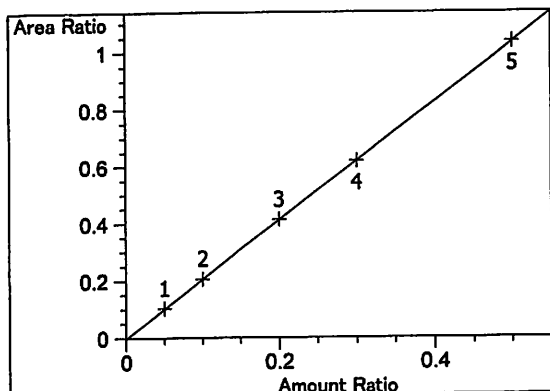


ethanol at exp. RT: 3.075  
 FID1 A, Front Signal  
 Correlation: 1.00000  
 Residual Std. Dev.: 0.00102  
 Formula:  $y = mx + b$   
 m: 2.07599  
 b: -2.10191e-3  
 x: Amount Ratio  
 y: Area Ratio

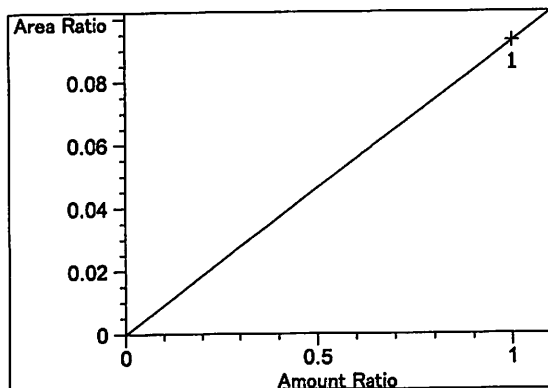


methanol at exp. RT: 3.388  
 FID2 B, Back Signal  
 Correlation: 1.00000  
 Residual Std. Dev.: 0.00000  
 Formula:  $y = mx + b$   
 m: 9.28944e-2  
 b: 0.00000  
 x: Amount Ratio  
 y: Area Ratio


W

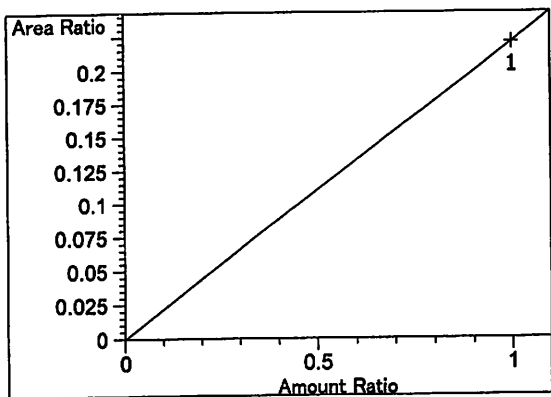


isopropyl alcohol at exp. RT: 3.628  
 FID1 A, Front Signal  
 Correlation: 1.00000  
 Residual Std. Dev.: 0.00000  
 Formula:  $y = mx + b$   
 m: 2.20737e-1  
 b: 0.00000  
 x: Amount Ratio  
 y: Area Ratio

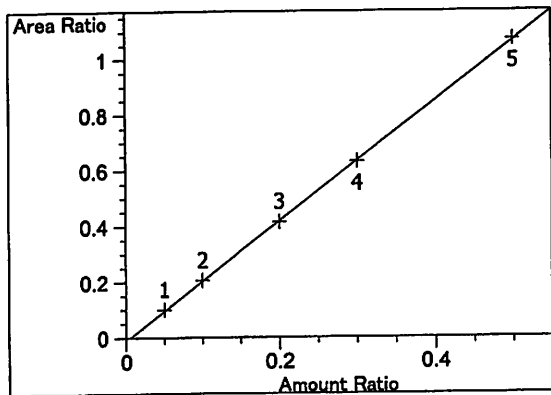

ethanol at exp. RT: 4.285  
 FID2 B, Back Signal  
 Correlation: 0.99994  
 Residual Std. Dev.: 0.00472  
 Formula:  $y = mx + b$   
 m: 2.15687  
 b: -1.08430e-2  
 x: Amount Ratio  
 y: Area Ratio

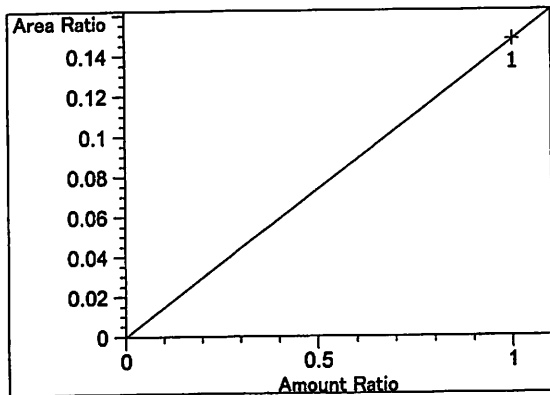


acetone at exp. RT: 4.308  
 FID1 A, Front Signal  
 Correlation: 1.00000  
 Residual Std. Dev.: 0.00000  
 Formula:  $y = mx + b$   
 m: 1.47439e-1  
 b: 0.00000  
 x: Amount Ratio  
 y: Area Ratio

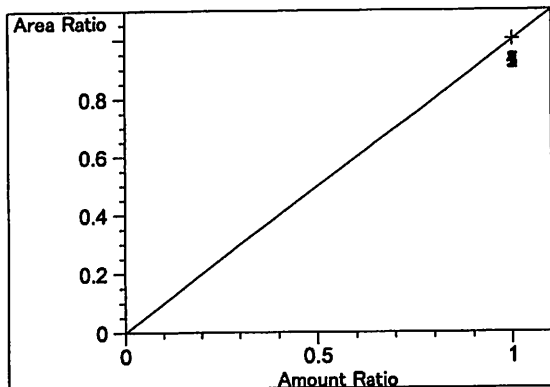


n-propanol at exp. RT: 4.620  
 FID1 A, Front Signal  
 Correlation: 1.00000  
 Residual Std. Dev.: 0.00000  
 Formula:  $y = mx + b$   
 m: 1.00000  
 b: 0.00000  
 x: Amount Ratio  
 y: Area Ratio


W

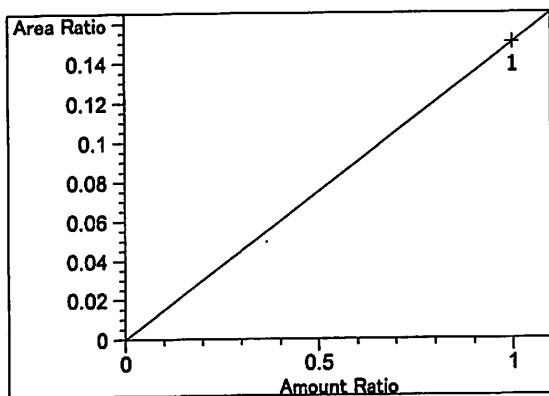

acetone at exp. RT: 4.661  
FID2 B, Back Signal  
Correlation: 1.00000  
Residual Std. Dev.: 0.00000  
Formula:  $y = mx + b$   
m: 1.50288e-1  
b: 0.00000  
x: Amount Ratio  
y: Area Ratio

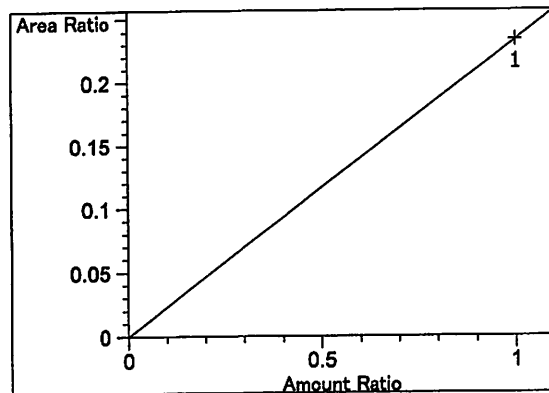

isopropyl alcohol at exp. RT: 4.969  
FID2 B, Back Signal  
Correlation: 1.00000  
Residual Std. Dev.: 0.00000  
Formula:  $y = mx + b$   
m: 2.33432e-1  
b: 0.00000  
x: Amount Ratio  
y: Area Ratio

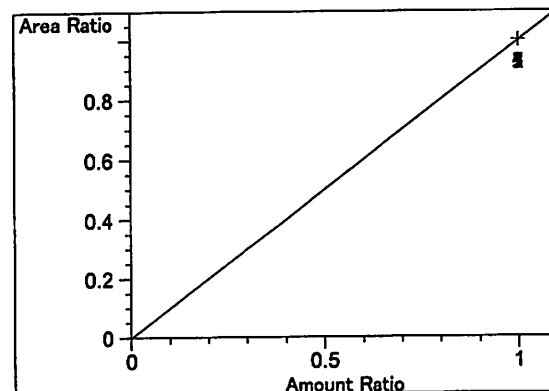

n-propanol at exp. RT: 7.550  
FID2 B, Back Signal  
Correlation: 1.00000  
Residual Std. Dev.: 0.00000  
Formula:  $y = mx + b$   
m: 1.00000  
b: 0.00000  
x: Amount Ratio  
y: Area Ratio


=====

W



ISP Forensic Services Blood Alcohol Report

Sample Name : 0.050 FN05211804  
 Laboratory : Meridian  
 Injection Date : Feb 5, 2020  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

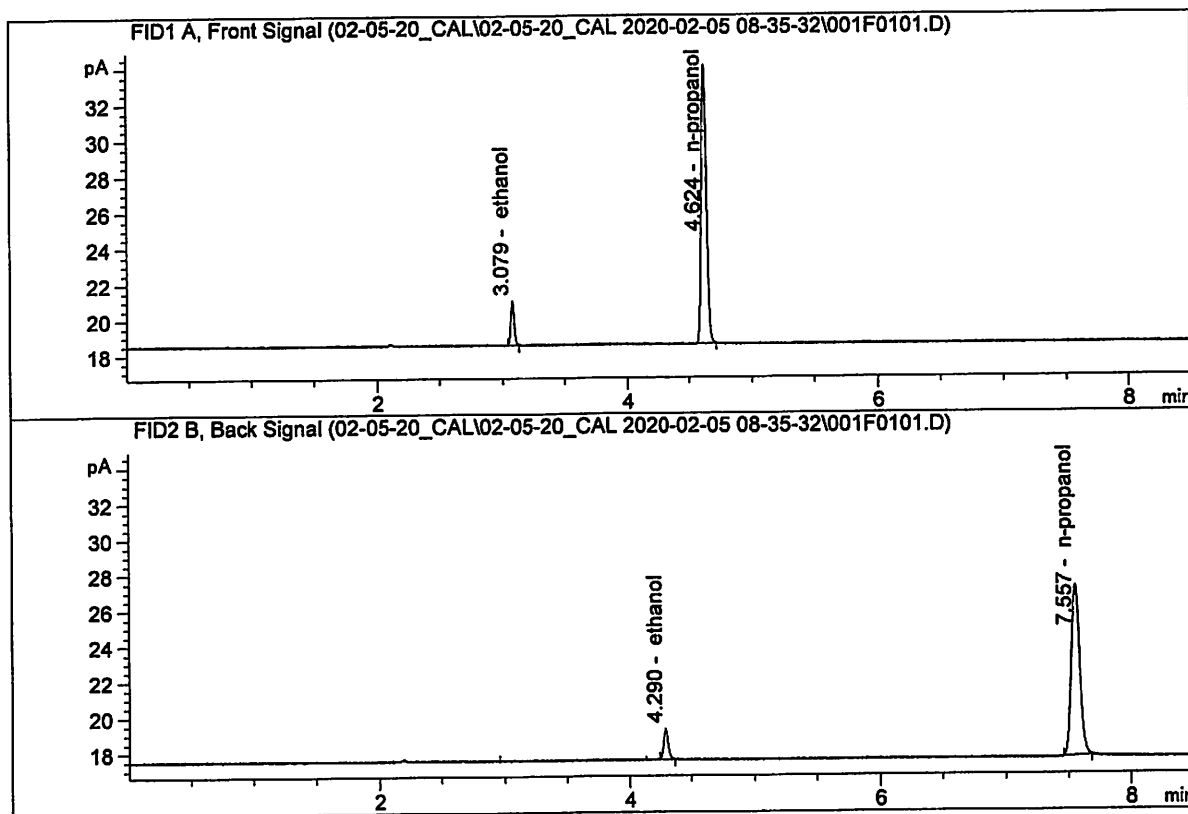


| #  | Compound   | Column    | Area     | Amount | Units   |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol    | Column 1: | 4.52242  | 0.0504 | g/100cc |
| 2. | Ethanol    | Column 2: | 4.62532  | 0.0518 | g/100cc |
| 3. | n-Propanol | Column 1: | 44.08209 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 45.86525 | 1.0000 | g/100cc |

*Handwritten mark*

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.100 FN02271802  
 Laboratory : Meridian  
 Injection Date : Feb 5, 2020  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

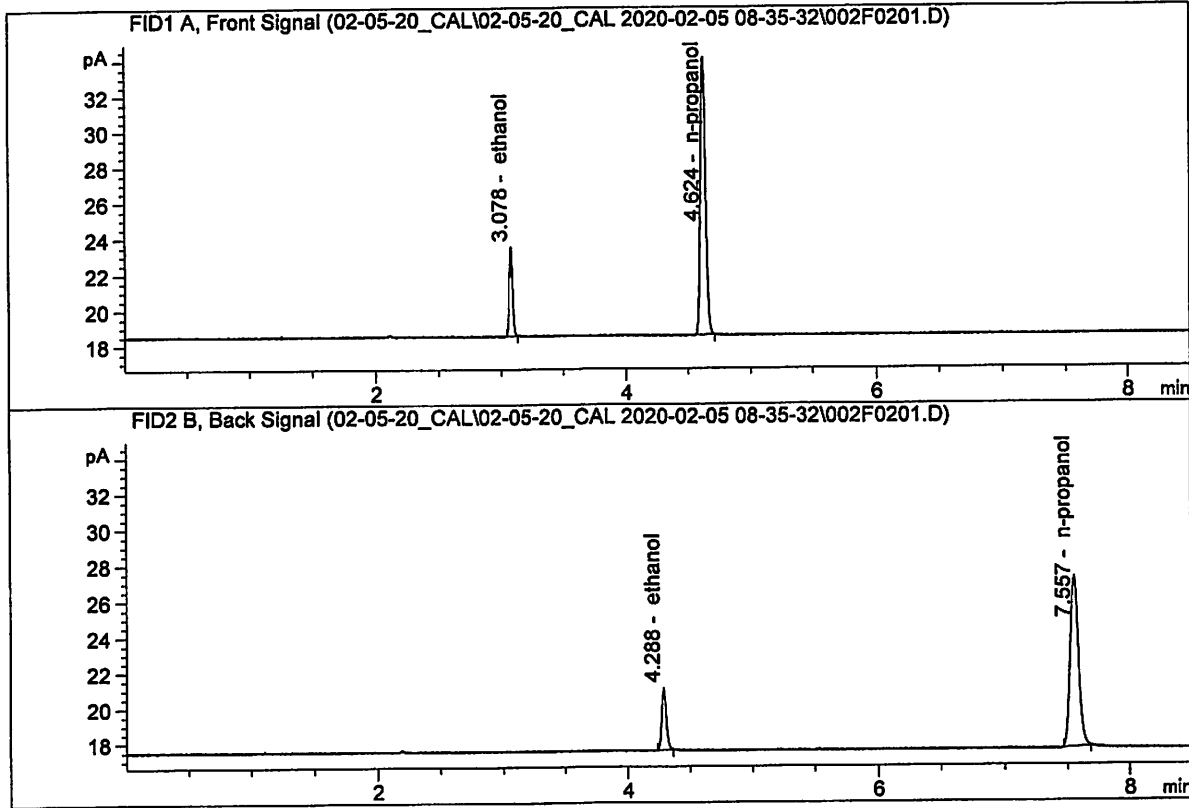


| #  | Compound   | Column    | Area     | Amount | Units   |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol    | Column 1: | 9.04952  | 0.0997 | g/100cc |
| 2. | Ethanol    | Column 2: | 9.39700  | 0.1005 | g/100cc |
| 3. | n-Propanol | Column 1: | 44.16013 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 45.63153 | 1.0000 | g/100cc |

*W*

# ISP Forensic Services Blood Alcohol Report

Sample Name : 0.200 FN06231704  
 Laboratory : Meridian  
 Injection Date : Feb 5, 2020  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

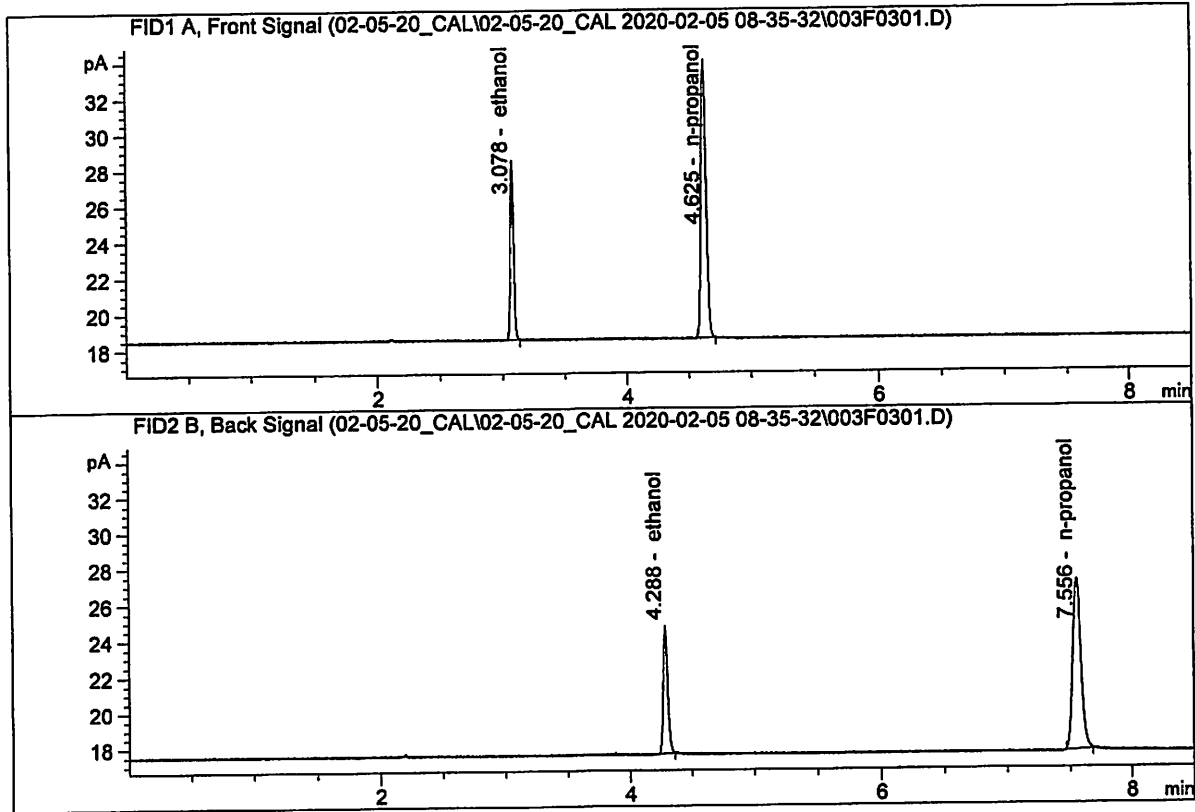


| #  | Compound   | Column    | Area     | Amount | Units   |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol    | Column 1: | 18.19493 | 0.2001 | g/100cc |
| 2. | Ethanol    | Column 2: | 18.84535 | 0.1980 | g/100cc |
| 3. | n-Propanol | Column 1: | 44.01959 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 45.28697 | 1.0000 | g/100cc |

*W*

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.300 FN07311804  
 Laboratory : Meridian  
 Injection Date : Feb 5, 2020  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

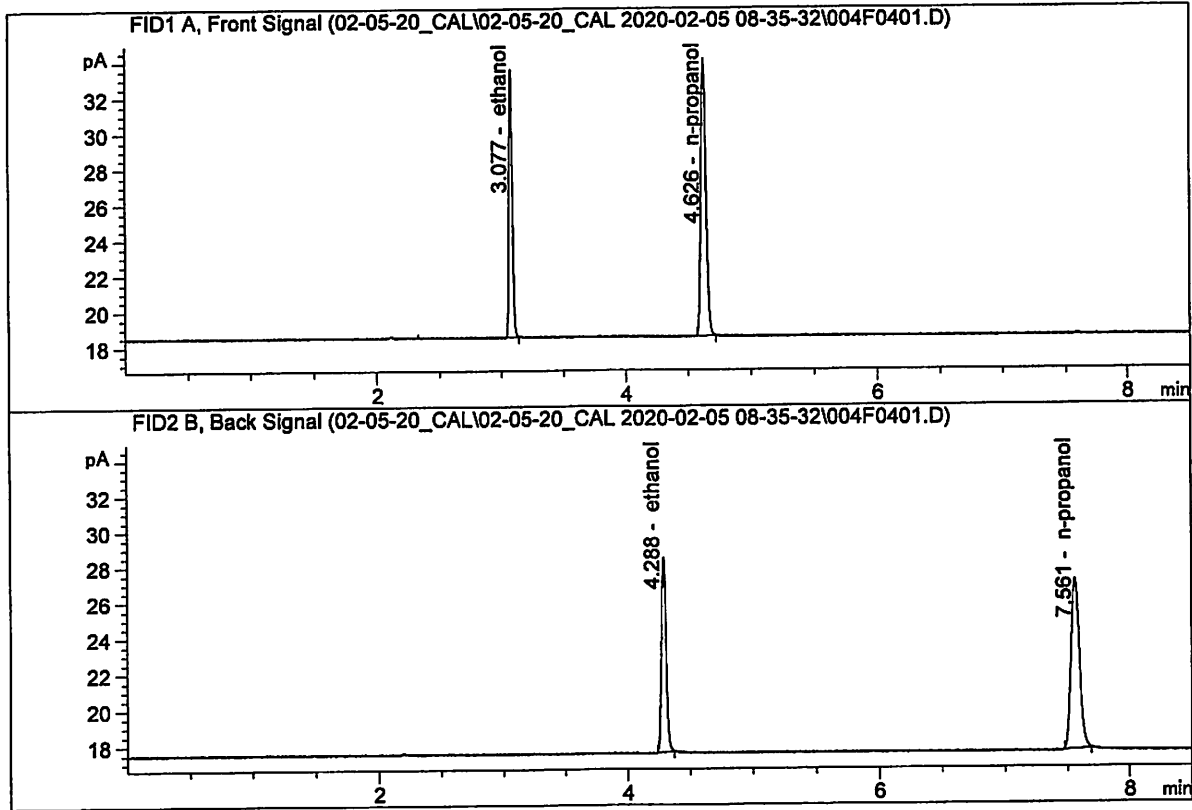


| #  | Compound   | Column    | Area     | Amount | Units   |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol    | Column 1: | 27.40895 | 0.2994 | g/100cc |
| 2. | Ethanol    | Column 2: | 28.70562 | 0.2980 | g/100cc |
| 3. | n-Propanol | Column 1: | 44.24614 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 45.42099 | 1.0000 | g/100cc |

W

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.500 FN08031602  
 Laboratory : Meridian  
 Injection Date : Feb 5, 2020  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

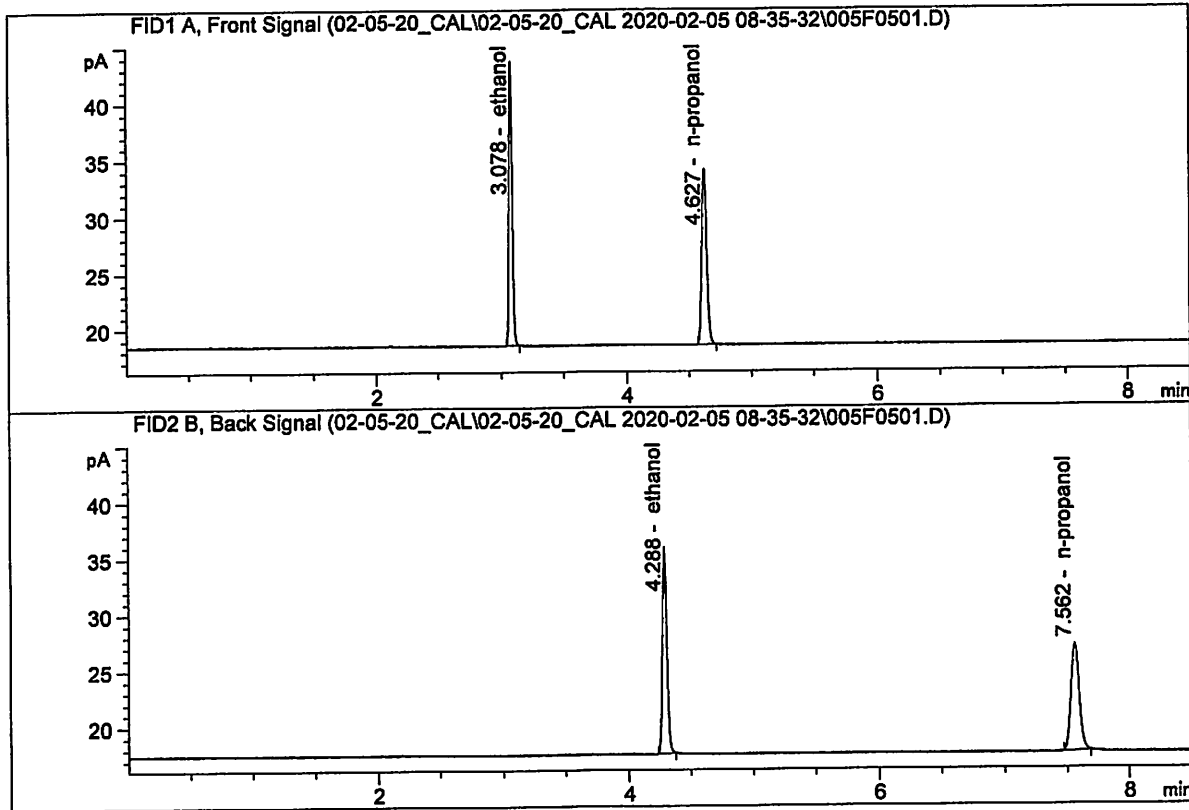


| #  | Compound   | Column    | Area     | Amount | Units   |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol    | Column 1: | 45.87756 | 0.5003 | g/100cc |
| 2. | Ethanol    | Column 2: | 48.52429 | 0.5017 | g/100cc |
| 3. | n-Propanol | Column 1: | 44.25955 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 45.29530 | 1.0000 | g/100cc |

*Handwritten signature*

ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STANDARD BLANK  
 Laboratory : Meridian  
 Injection Date : Feb 5, 2020  
 Method : ALCOHOL.M  
 Acq. Instrument: CN11180014-CN11041167

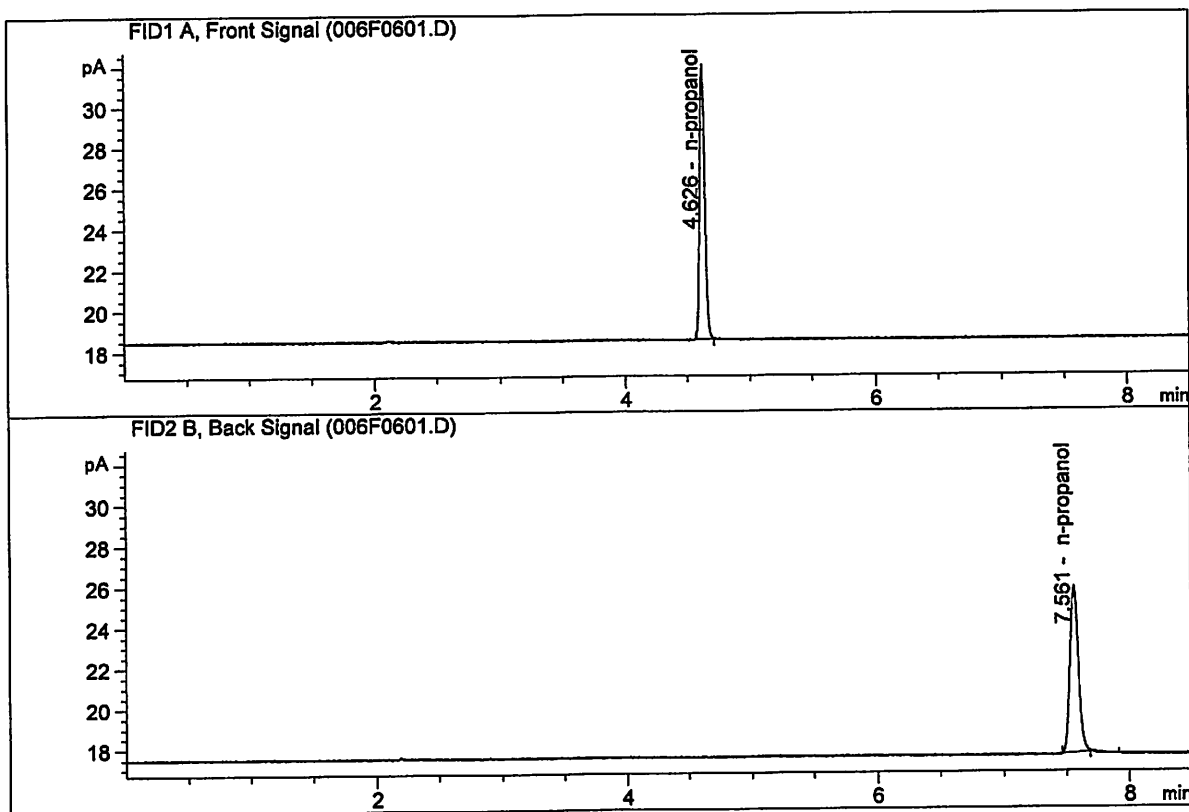

| #  | Compound   | Column    | Area     | Amount | Units   |
|----|------------|-----------|----------|--------|---------|
| 1. | Ethanol    | Column 1: | 0.00000  | 0.0000 | g/100cc |
| 2. | Ethanol    | Column 2: | 0.00000  | 0.0000 | g/100cc |
| 3. | n-Propanol | Column 1: | 38.32483 | 1.0000 | g/100cc |
| 4. | n-Propanol | Column 2: | 39.03453 | 1.0000 | g/100cc |

*W*

S a m p l e S u m m a r y

Sequence table: C:\Chem32\1\Data\02-05-20\_CAL\02-05-20\_CAL 2020-02-05 08-35-32\02-05-20\_CAL.S  
 Data directory path: C:\Chem32\1\Data\02-05-20\_CAL\02-05-20\_CAL 2020-02-05 08-35-32\  
 Logbook: C:\Chem32\1\Data\02-05-20\_CAL\02-05-20\_CAL 2020-02-05 08-35-32\02-05-20\_CAL.LOG  
 Sequence start: 2/5/2020 8:50:11 AM  
 Sequence Operator: SYSTEM  
 Operator: SYSTEM

Method file name: C:\Chem32\1\Data\02-05-20\_CAL\02-05-20\_CAL 2020-02-05 08-35-32\ALCOHOL.M

| Run # | Location # | Inj # | Sample Name      | Sample Amt [g/100cc] | Multip.* Dilution | File name  | Cal # | # Cmp |
|-------|------------|-------|------------------|----------------------|-------------------|------------|-------|-------|
| 1     | 1          | 1     | 0.050 FN05211804 | -                    | 1.0000            | 001F0101.D | *     | 4     |
| 2     | 2          | 1     | 0.100 FN02271802 | -                    | 1.0000            | 002F0201.D | *     | 4     |
| 3     | 3          | 1     | 0.200 FN06231704 | -                    | 1.0000            | 003F0301.D | *     | 4     |
| 4     | 4          | 1     | 0.300 FN07311804 | -                    | 1.0000            | 004F0401.D | *     | 4     |
| 5     | 5          | 1     | 0.500 FN08031602 | -                    | 1.0000            | 005F0501.D | *     | 4     |
| 6     | 6          | 1     | INTERNAL STANDAR | -                    | 1.0000            | 006F0601.D |       | 2     |