

Quantitative Analysis for Ethanol & Qualitative Analysis for Other Volatiles

Analytical Method(s): 1.0

Device: Hamilton MICROLAB Liquid Processor/Dilutor Serial Number: ML600HC11378 MB

11/19/20

Volatiles Quality Assurance Controls Run Date(s): 11/18/20-11/19/2020

calibration: 11/6/20

Control level	Expiration	Lot #	Target Value	Acceptable Range	Overall Results
Level 1	Jul-23	1907006	0.0764	0.0688-0.0840	0.0741 g/100cc
					0.0757 g/100cc
					g/100cc
Level 2	Mar-22	1803028	0.2035	0.1832-0.2238	0.2043 g/100cc
					0.2071 g/100cc
Multi-Component mixture:					
Curve Fit:		Column 1	Lot #	Column 2	
		0.99999	FN07101701	0.99991	acceptable

Ethanol Calibration Reference Material						
Calibrator level	Target Value	Acceptable Range	Column 1	Column 2	Precision	Mean
50	0.050	0.045 - 0.055	0.0510	0.0527	0.0017	0.0518
100	0.100	0.090 - 0.110	0.1001	0.0999	0.0002	0.1
200	0.200	0.180 - 0.220	0.1989	0.1975	0.0014	0.1982
300	0.300	0.270 - 0.330	0.2992	0.2978	0.0014	0.2985
400	0.400	0.360 - 0.440			0	#DIV/0!
500	0.500	0.450 - 0.550	0.5008	0.5021	0.0013	0.5014


Aqueous Controls			
Control level	Target Value	Acceptable Range	Overall Results
80	0.080	0.076 - 0.084	0.082 g/100cc

REVIEWED

By Galina Giso at 9:58 am, Nov 19, 2020

Worklist: 4613

<u>LAB CASE</u>	<u>ITEM</u>	<u>ITEM TYPE</u>	<u>DESCRIPTION</u>
M2020-0952	16	BLOOD	Alcohol Analysis
M2020-4564	1	BCK	Alcohol Analysis
M2020-4565	1	BCK	Alcohol Analysis
M2020-4577	2	BCK	Alcohol Analysis
M2020-4585	1	BCK	Alcohol Analysis
M2020-4586	1	BCK	Alcohol Analysis
M2020-4594	1	BCK	Alcohol Analysis
M2020-4614	1	BCK	Alcohol Analysis
M2020-4617	1	BCK	Alcohol Analysis
M2020-4626	1	BCK	Alcohol Analysis
M2020-4630	2	BCK	Alcohol Analysis
M2020-4667	1	BCK	Alcohol Analysis
M2020-4668	1	BCK	Alcohol Analysis
M2020-4670	1	BCK	Alcohol Analysis
M2020-4671	1	BCK	Alcohol Analysis
M2020-4672	1	BCK	Alcohol Analysis
M2020-4673	1	BCK	Alcohol Analysis
M2020-4680	1	BCK	Alcohol Analysis
M2020-4687	1	BCK	Alcohol Analysis
M2020-4688	1	BCK	Alcohol Analysis
M2020-4689	1	BCK	Alcohol Analysis

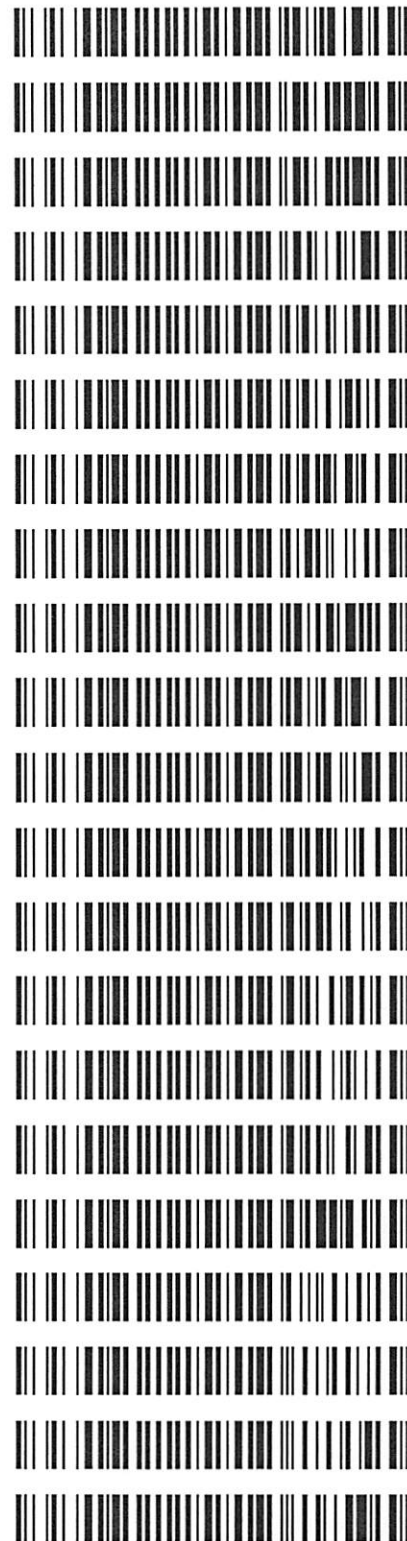

NB

=====
Calibration Table
=====

General Calibration Setting

Calib. Data Modified : Friday, November 06, 2020 12:08:12 PM
Signals calculated separately : No

Rel. Reference Window : 0.000 %
Abs. Reference Window : 0.100 min
Rel. Non-ref. Window : 0.000 %
Abs. Non-ref. Window : 0.100 min
Uncalibrated Peaks : not reported
Partial Calibration : Yes, identified peaks are recalibrated
Correct All Ret. Times: No, only for identified peaks

Curve Type : Linear
Origin : Ignored
Weight : Equal

Recalibration Settings:
Average Response : Average all calibrations
Average Retention Time: Floating Average New 75%

Calibration Report Options :
Printout of recalibrations within a sequence:
 Calibration Table after Recalibration
 Normal Report after Recalibration
If the sequence is done with bracketing:
 Results of first cycle (ending previous bracket)

Default Sample ISTD Information (if not set in sample table):

ISTD #	ISTD Amount [g/100cc]	Name
1	1.00000	n-propanol
2	1.00000	n-propanol

Signal Details

Signal 1: FID1 A, Front Signal
Signal 2: FID2 B, Back Signal

Overview Table

RT	Sig	Lvl	Amount [g/100cc]	Area	Rsp.Factor	Ref	ISTD #	Compound
2.586	1	1	1.00000	3.69669	2.70512e-1	No	No 1	methanol
2.809	1	1	1.00000	4.26100	2.34687e-1	No	No 2	Acetaldehyde
2.977	2	1	1.00000	4.26100	2.34687e-1	No	No 2	Acetaldehyde
3.075	1	1	5.00000e-2	4.49381	1.11264e-2	No	No 1	ethanol
			1.00000e-1	8.93291	1.11946e-2			
			2.00000e-1	17.78029	1.12484e-2			
			3.00000e-1	26.94336	1.11345e-2			
			5.00000e-1	44.95221	1.11229e-2			
3.388	2	1	1.00000	4.26062	2.34707e-1	No	No 2	methanol
3.628	1	1	1.00000	9.73055	1.02769e-1	No	No 1	isopropyl alcohol
4.285	2	1	5.00000e-2	4.60429	1.08594e-2	No	No 2	ethanol
			1.00000e-1	9.11517	1.09707e-2			
			2.00000e-1	18.34945	1.08995e-2			
			3.00000e-1	28.10586	1.06739e-2			
			5.00000e-1	47.23547	1.05853e-2			
4.308	1	1	1.00000	6.49940	1.53860e-1	No	No 1	acetone
4.620	1	1	1.00000	46.99450	2.12791e-2	No	Yes 1	n-propanol
			1.00000	46.60860	2.14553e-2			
			1.00000	46.19387	2.16479e-2			
			1.00000	46.35681	2.15718e-2			
			1.00000	46.07421	2.17041e-2			
4.661	2	1	1.00000	6.89301	1.45075e-1	No	No 2	acetone
4.969	2	1	1.00000	10.70642	9.34019e-2	No	No 2	isopropyl alcohol
7.550	2	1	1.00000	48.71027	2.05295e-2	No	Yes 2	n-propanol
			1.00000	47.93089	2.08634e-2			
			1.00000	47.28535	2.11482e-2			
			1.00000	47.53572	2.10368e-2			
			1.00000	46.98842	2.12818e-2			


Peak Sum Table

No Entries in table

1 Warnings or Errors :


Warning : Curve requires more calibration points., (methanol)

Calibration Curves

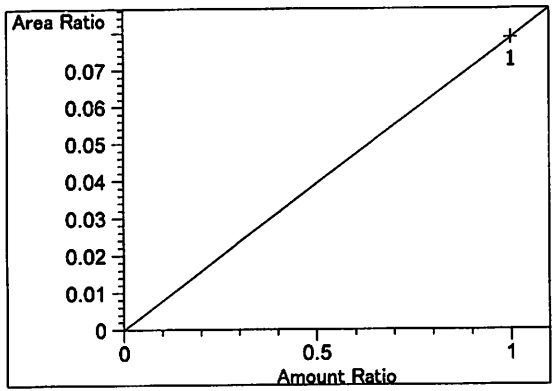


methanol at exp. RT: 2.586
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 7.86623e-2
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio


NB

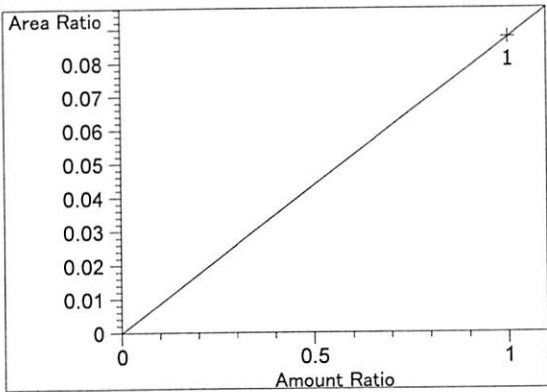


Acetaldehyde at exp. RT: 2.809
FID1 A, Front Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx + b$
m: $8.74764e-2$
b: 0.00000
x: Amount Ratio
y: Area Ratio

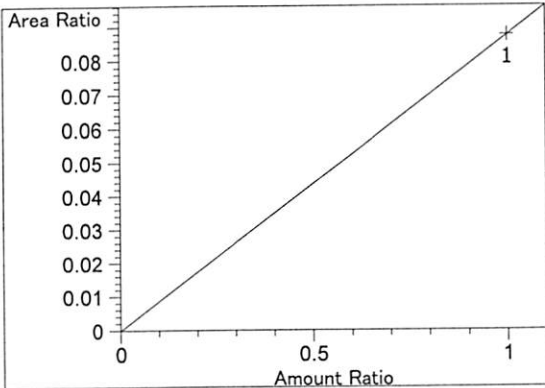

Acetaldehyde at exp. RT: 2.977
FID2 B, Back Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx + b$
m: $8.74764e-2$
b: 0.00000
x: Amount Ratio
y: Area Ratio

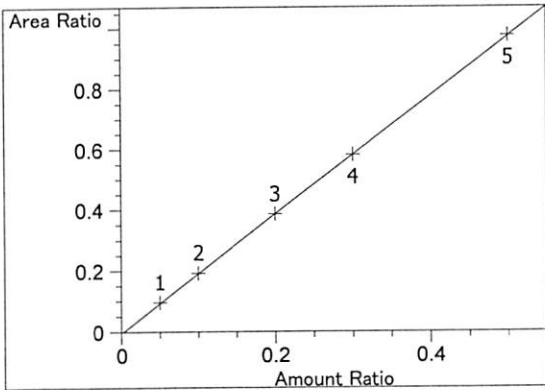


ethanol at exp. RT: 3.075
FID1 A, Front Signal
Correlation: 0.99999 *
Residual Std. Dev.: 0.00214
Formula: $y = mx + b$
m: 1.95652
b: $-4.18994e-3$
x: Amount Ratio
y: Area Ratio

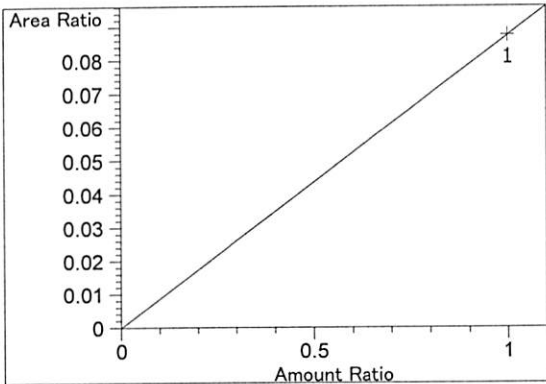


methanol at exp. RT: 3.388
FID2 B, Back Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx + b$
m: $8.74687e-2$
b: 0.00000
x: Amount Ratio
y: Area Ratio


NB

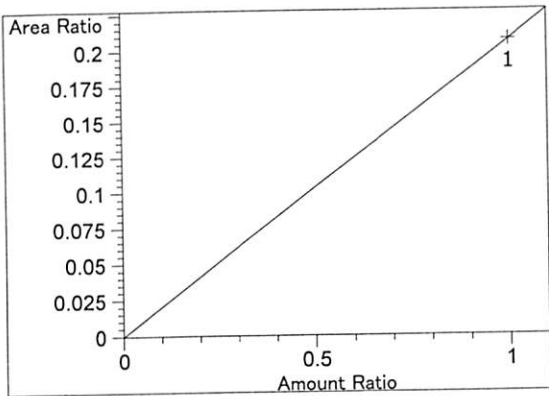


isopropyl alcohol at exp. RT: 3.628
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 2.07057e-1
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio

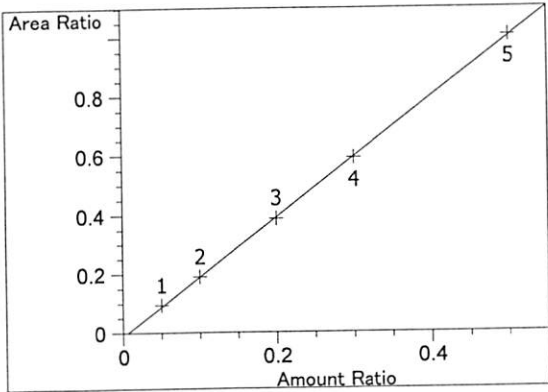

ethanol at exp. RT: 4.285
 FID2 B, Back Signal
 Correlation: 0.99991
 Residual Std. Dev.: 0.00555
 Formula: $y = mx + b$
 m: 2.02679
 b: -1.23075e-2
 x: Amount Ratio
 y: Area Ratio

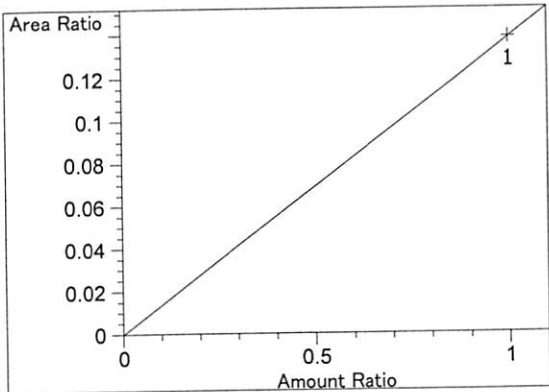


acetone at exp. RT: 4.308
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 1.38301e-1
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio

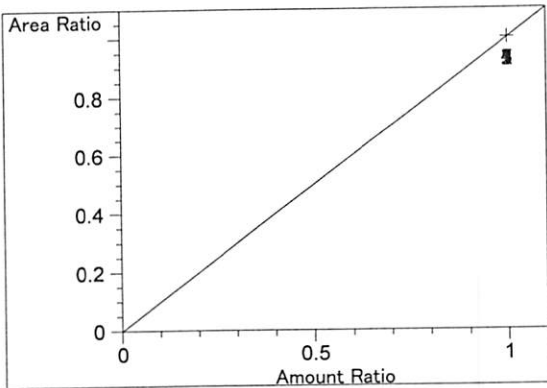


n-propanol at exp. RT: 4.620
 FID1 A, Front Signal
 Correlation: 1.00000
 Residual Std. Dev.: 0.00000
 Formula: $y = mx + b$
 m: 1.00000
 b: 0.00000
 x: Amount Ratio
 y: Area Ratio


MB

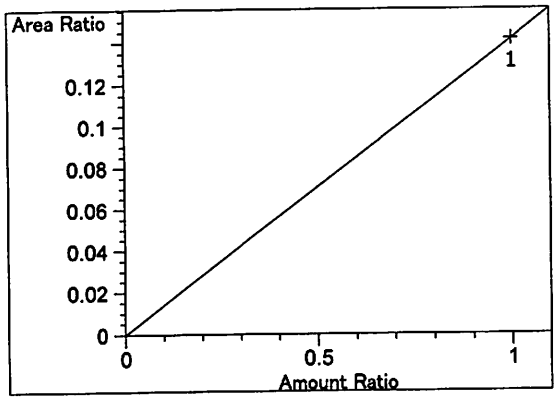

acetone at exp. RT: 4.661
FID2 B, Back Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx + b$
m: 1.41510e-1
b: 0.00000
x: Amount Ratio
y: Area Ratio

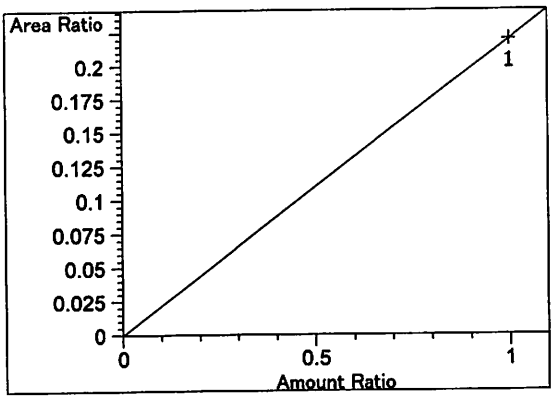

isopropyl alcohol at exp. RT: 4.969
FID2 B, Back Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx + b$
m: 2.19798e-1
b: 0.00000
x: Amount Ratio
y: Area Ratio

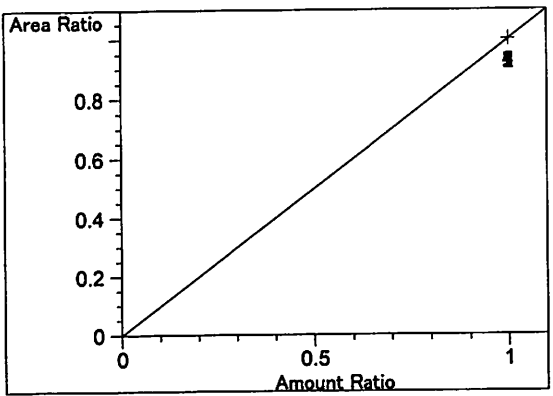


n-propanol at exp. RT: 7.550
FID2 B, Back Signal
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx + b$
m: 1.00000
b: 0.00000
x: Amount Ratio
y: Area Ratio

=====

NB

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.050 FN05211804
 Laboratory : Meridian
 Injection Date : Nov 6, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

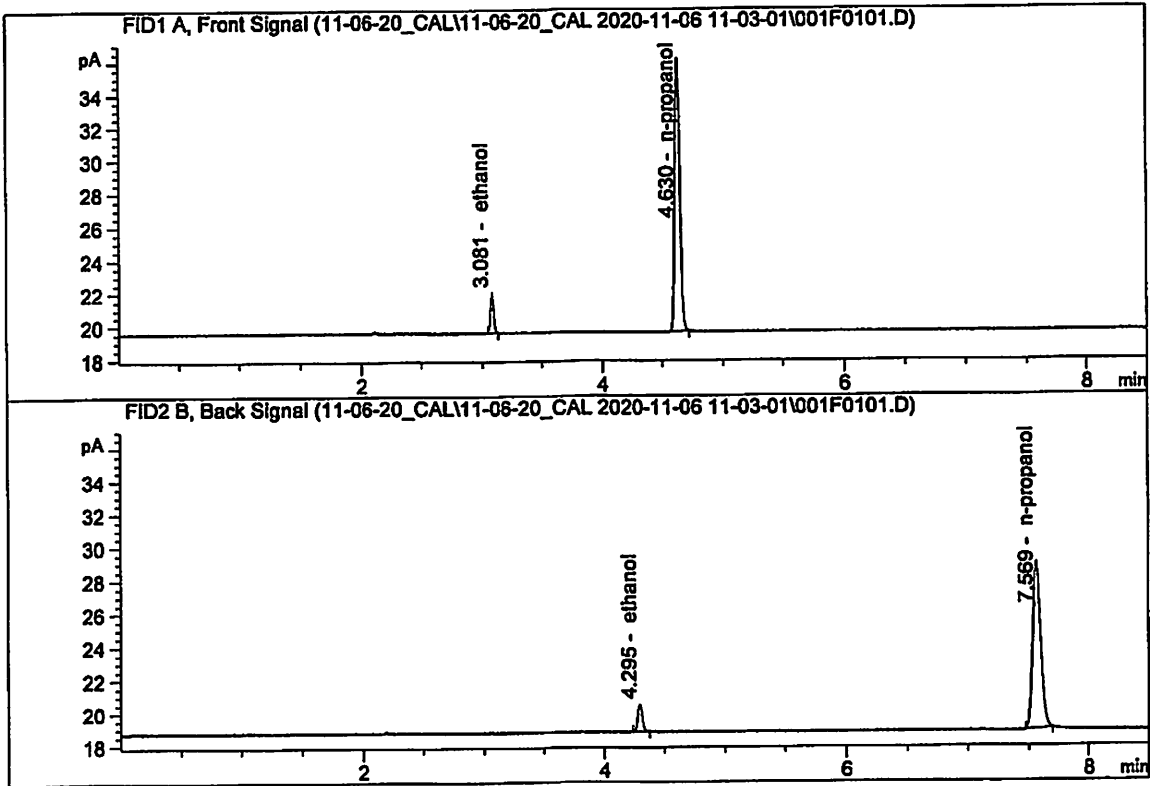


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	4.49381	0.0510	g/100cc
2.	Ethanol	Column 2:	4.60429	0.0527	g/100cc
3.	n-Propanol	Column 1:	46.99450	1.0000	g/100cc
4.	n-Propanol	Column 2:	48.71027	1.0000	g/100cc

NB

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.100 FN02271802
 Laboratory : Meridian
 Injection Date : Nov 6, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

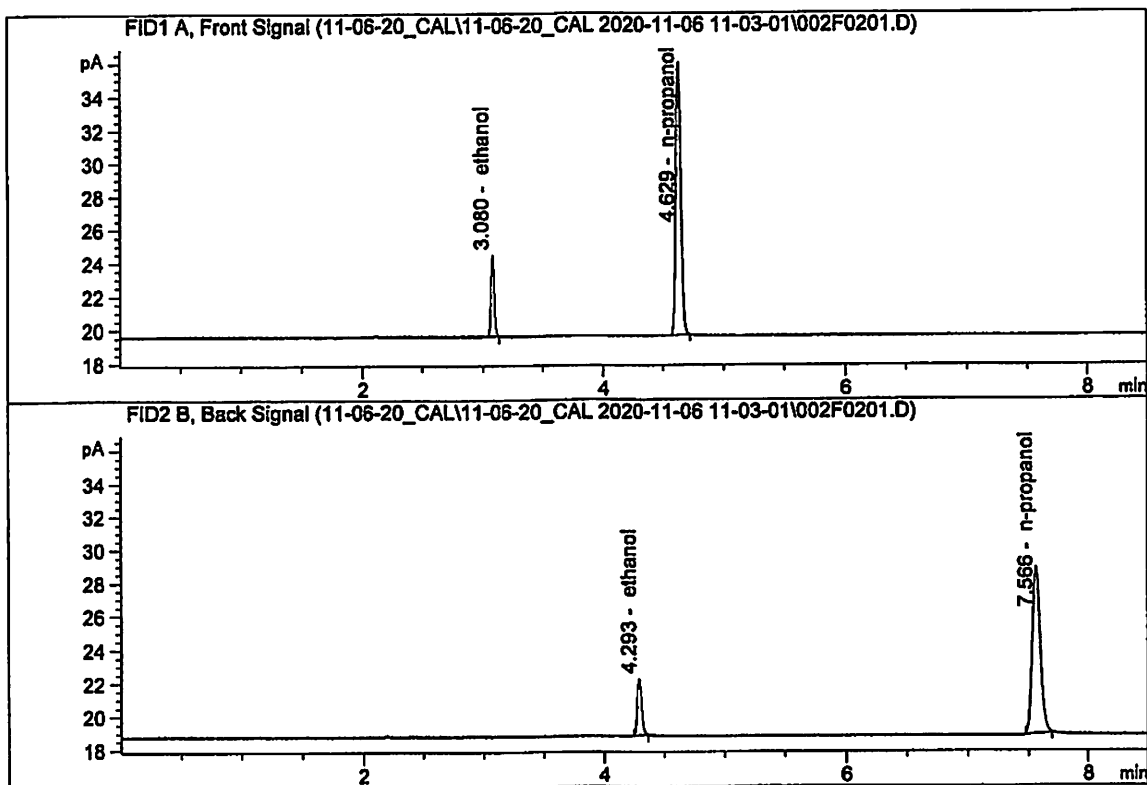


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	8.93291	0.1001	g/100cc
2.	Ethanol	Column 2:	9.11517	0.0999	g/100cc
3.	n-Propanol	Column 1:	46.60860	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.93089	1.0000	g/100cc

NB

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.200 FN06231704
 Laboratory : Meridian
 Injection Date : Nov 6, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

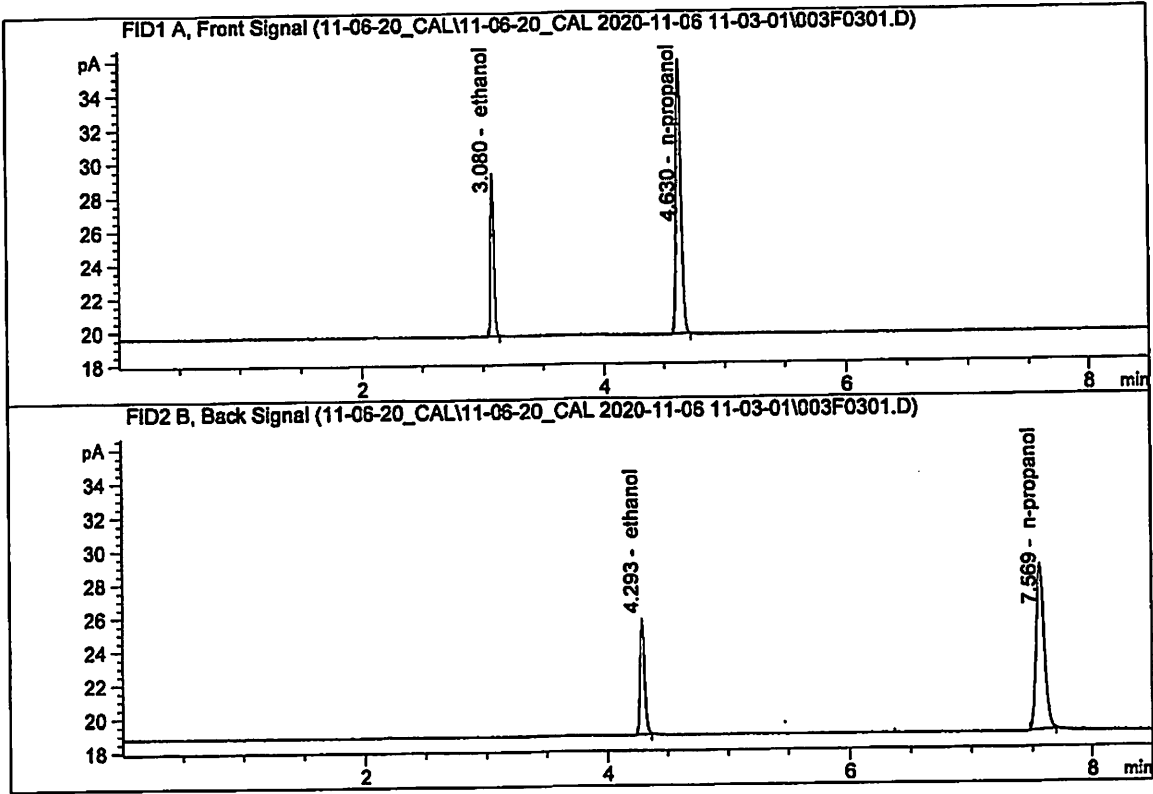


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	17.78029	0.1989	g/100cc
2.	Ethanol	Column 2:	18.34945	0.1975	g/100cc
3.	n-Propanol	Column 1:	46.19387	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.28535	1.0000	g/100cc

NB

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.300 FN07311804
 Laboratory : Meridian
 Injection Date : Nov 6, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

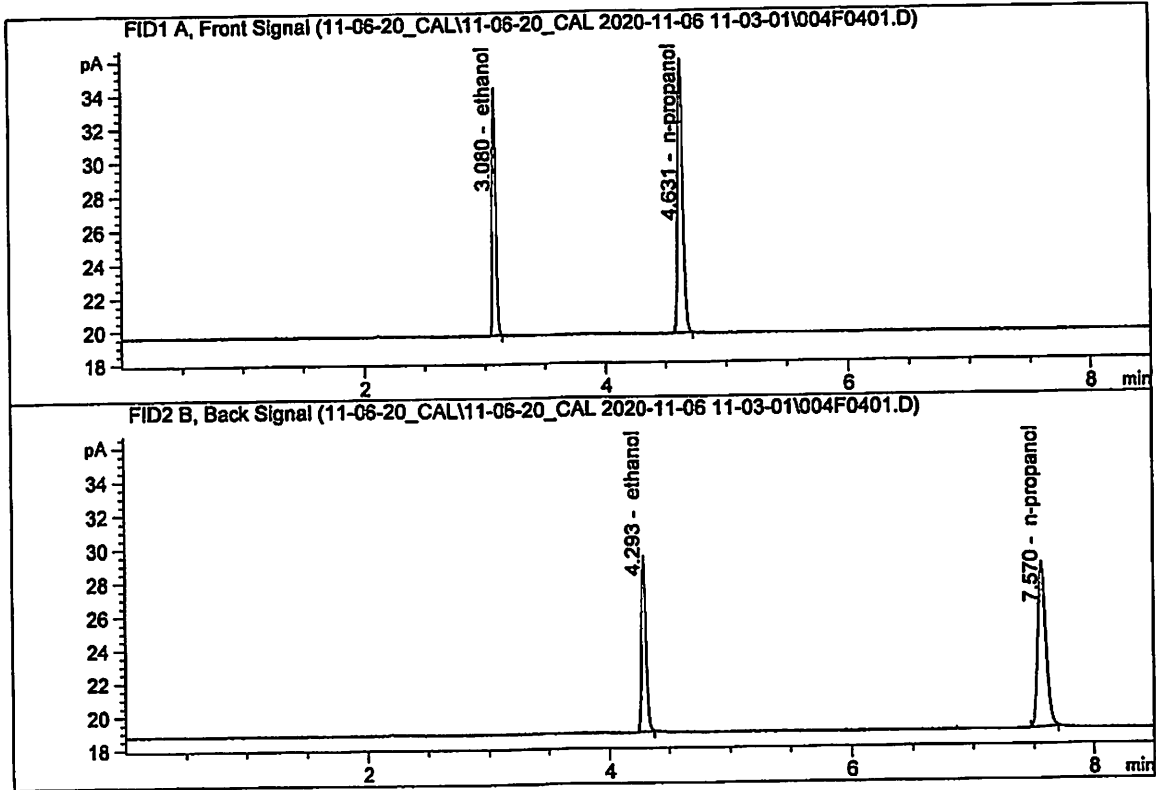


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	26.94336	0.2992	g/100cc
2.	Ethanol	Column 2:	28.10586	0.2978	g/100cc
3.	n-Propanol	Column 1:	46.35681	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.53572	1.0000	g/100cc

NB

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.500 FN08241801
 Laboratory : Meridian
 Injection Date : Nov 6, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

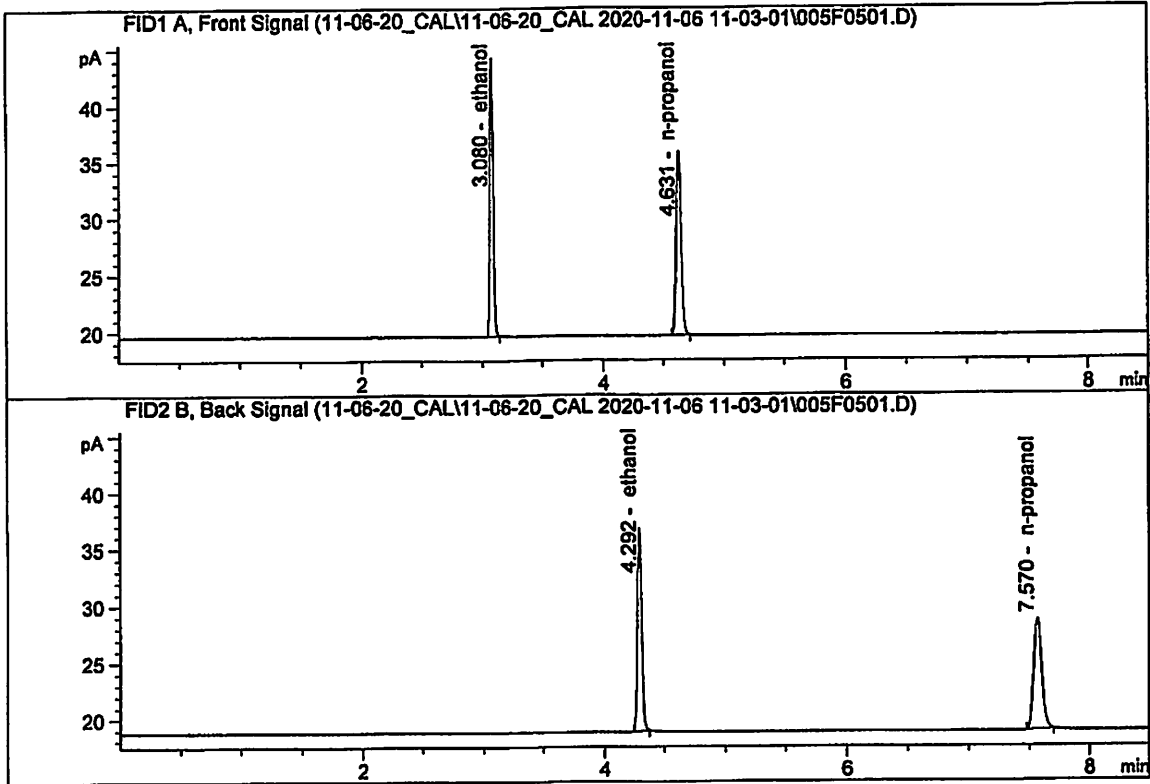


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	44.95221	0.5008	g/100cc
2.	Ethanol	Column 2:	47.23547	0.5021	g/100cc
3.	n-Propanol	Column 1:	46.07421	1.0000	g/100cc
4.	n-Propanol	Column 2:	46.98842	1.0000	g/100cc

NB

ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STANDARD BLANK
 Laboratory : Meridian
 Injection Date : Nov 6, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

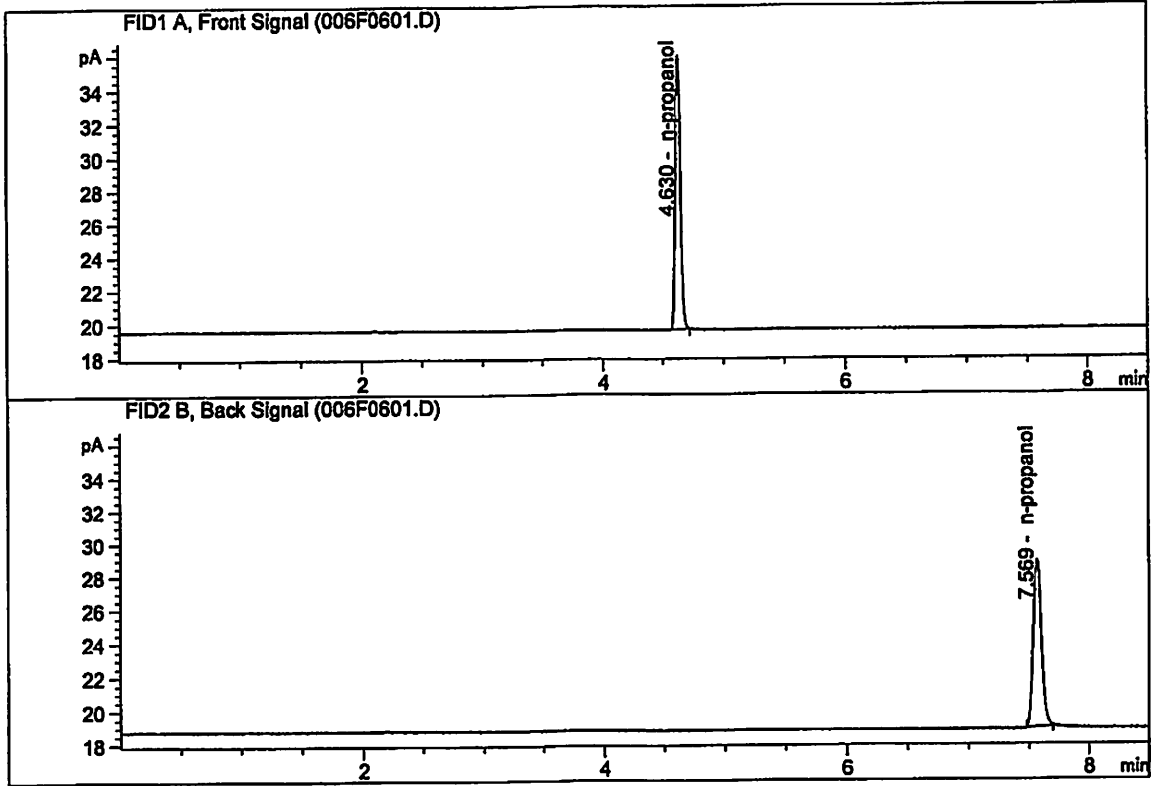

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	46.43234	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.34886	1.0000	g/100cc

NB

S a m p l e S u m m a r y


Sequence table: C:\Chem32\1\Data\11-06-20_CAL\11-06-20_CAL 2020-11-06 11-03-01\11-06-20_CAL.S
 Data directory path: C:\Chem32\1\Data\11-06-20_CAL\11-06-20_CAL 2020-11-06 11-03-01\
 Logbook: C:\Chem32\1\Data\11-06-20_CAL\11-06-20_CAL 2020-11-06 11-03-01\11-06-20_CAL.LOG
 Sequence start: 11/6/2020 11:17:40 AM
 Sequence Operator: SYSTEM
 Operator: SYSTEM
 Method file name: C:\Chem32\1\Data\11-06-20_CAL\11-06-20_CAL 2020-11-06 11-03-01\ALCOHOL.M

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #	Cmp
1	1	1	0.050 FN05211804	-	1.0000	001F0101.D	*	4
2	2	1	0.100 FN02271802	-	1.0000	002F0201.D	*	4
3	3	1	0.200 FN06231704	-	1.0000	003F0301.D	*	4
4	4	1	0.300 FN07311804	-	1.0000	004F0401.D	*	4
5	5	1	0.500 FN08241801	-	1.0000	005F0501.D	*	4
6	6	1	INTERNAL STANDAR	-	1.0000	006F0601.D		2

NB

ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STD BLK 1
 Laboratory : Meridian
 Injection Date : Nov 18, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

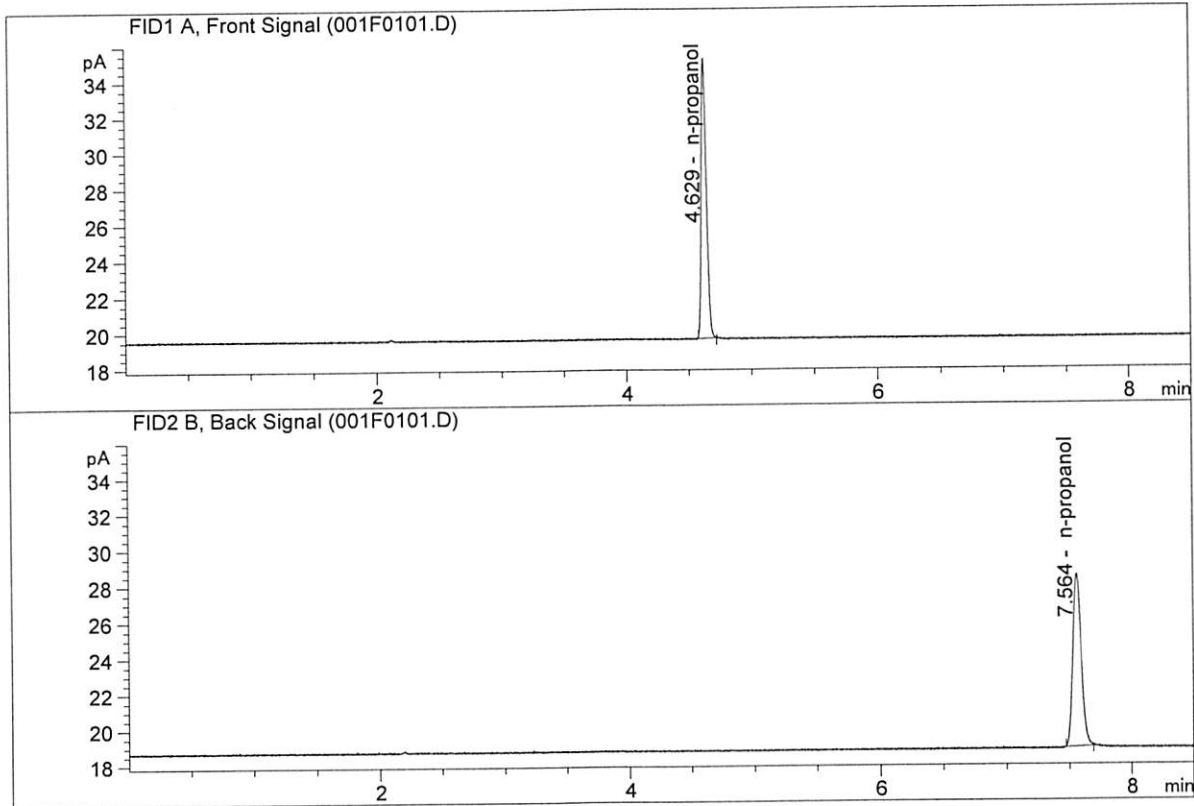


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	44.40253	1.0000	g/100cc
4.	n-Propanol	Column 2:	46.19690	1.0000	g/100cc

NB

ISP Forensic Services Blood Alcohol Report

Sample Name : MIX VOL FN007101701
 Laboratory : Meridian
 Injection Date : Nov 18, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

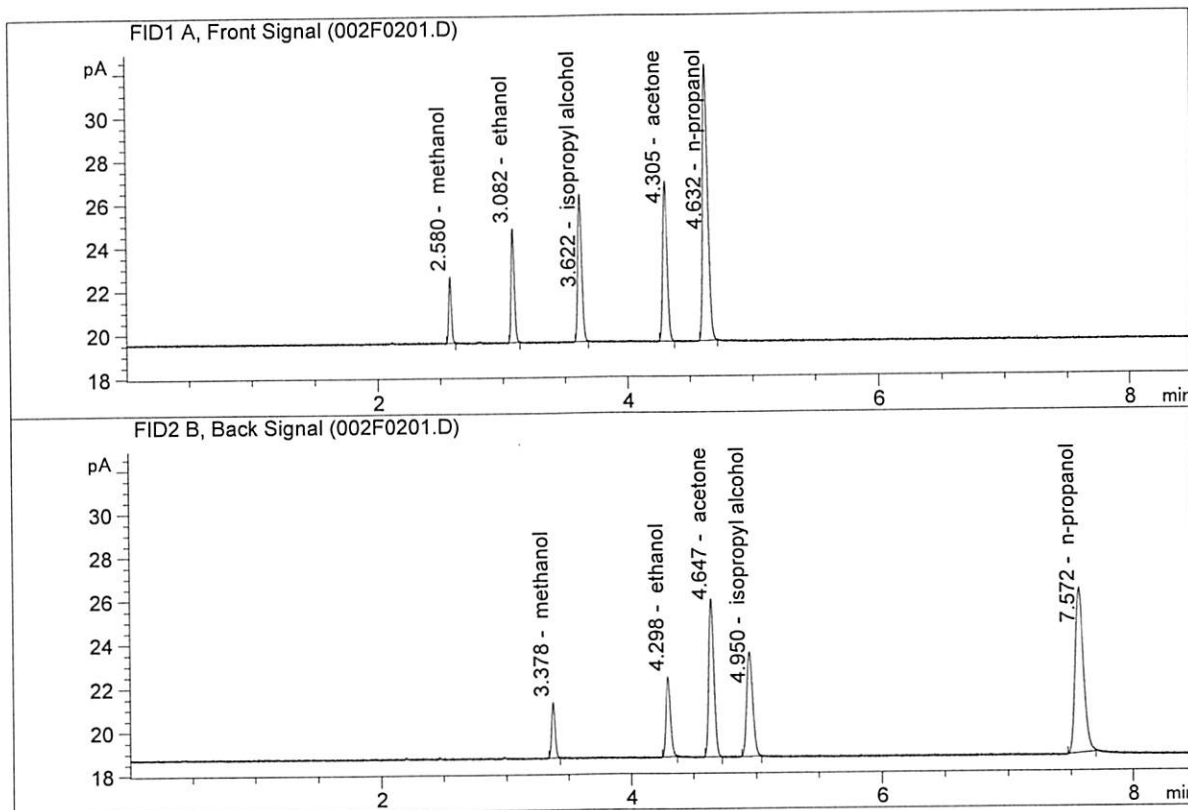

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	9.21910	0.1352	g/100cc
2.	Ethanol	Column 2:	9.56139	0.1372	g/100cc
3.	n-Propanol	Column 1:	35.42504	1.0000	g/100cc
4.	n-Propanol	Column 2:	35.96337	1.0000	g/100cc

NB

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC1-1

Analysis Date(s): 18 Nov 2020

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Sample A-B Difference	Over-all Mean
Sample Results	0.0738	0.0752	0.0014	0.0745	0.0007	0.0741
(g/100cc)	0.0732	0.0745	0.0013	0.0738		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument information is stored centrally.

Refer to Instrument Method: Alcohol.m

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.074	0.070	0.078	0.004


	Reported Result	
	0.074	

Calibration and control data are stored centrally.

NB

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-1-A
 Laboratory : Meridian
 Injection Date : Nov 18, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

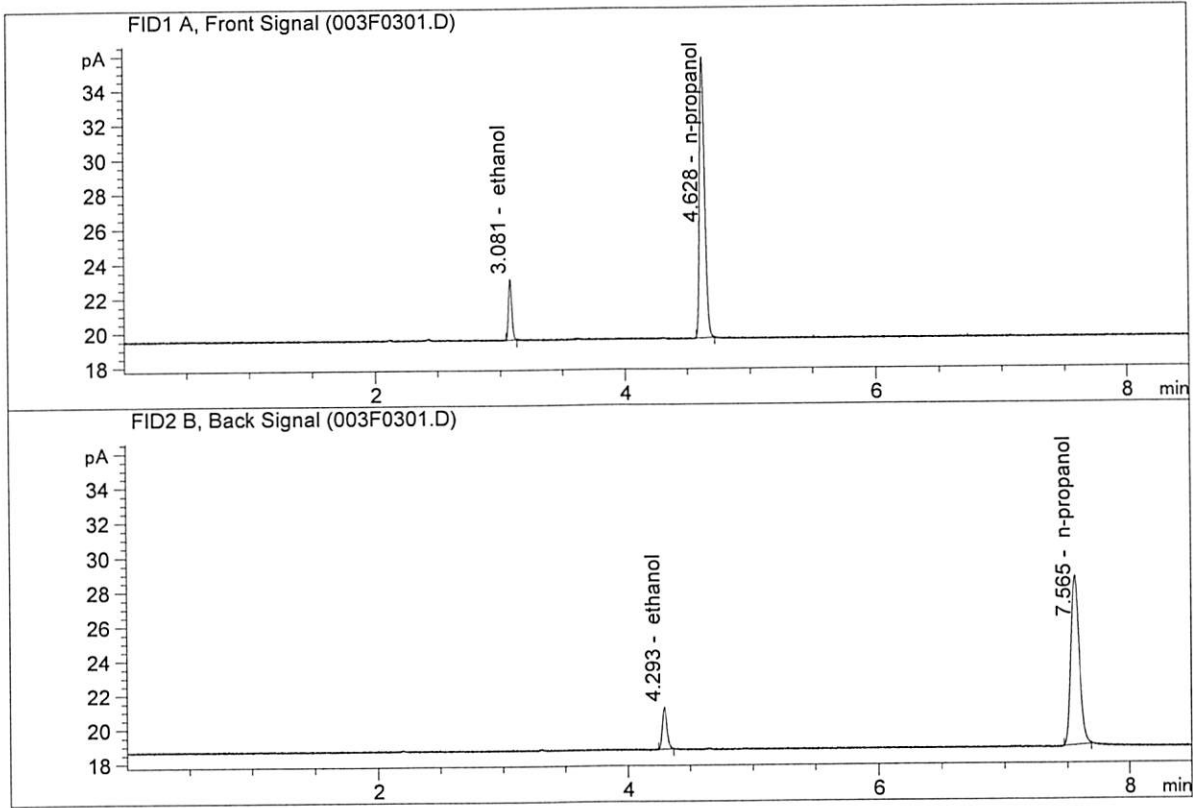


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	6.46541	0.0738	g/100cc
2.	Ethanol	Column 2:	6.60512	0.0752	g/100cc
3.	n-Propanol	Column 1:	46.13480	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.14452	1.0000	g/100cc

NB

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-1-B
 Laboratory : Meridian
 Injection Date : Nov 18, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

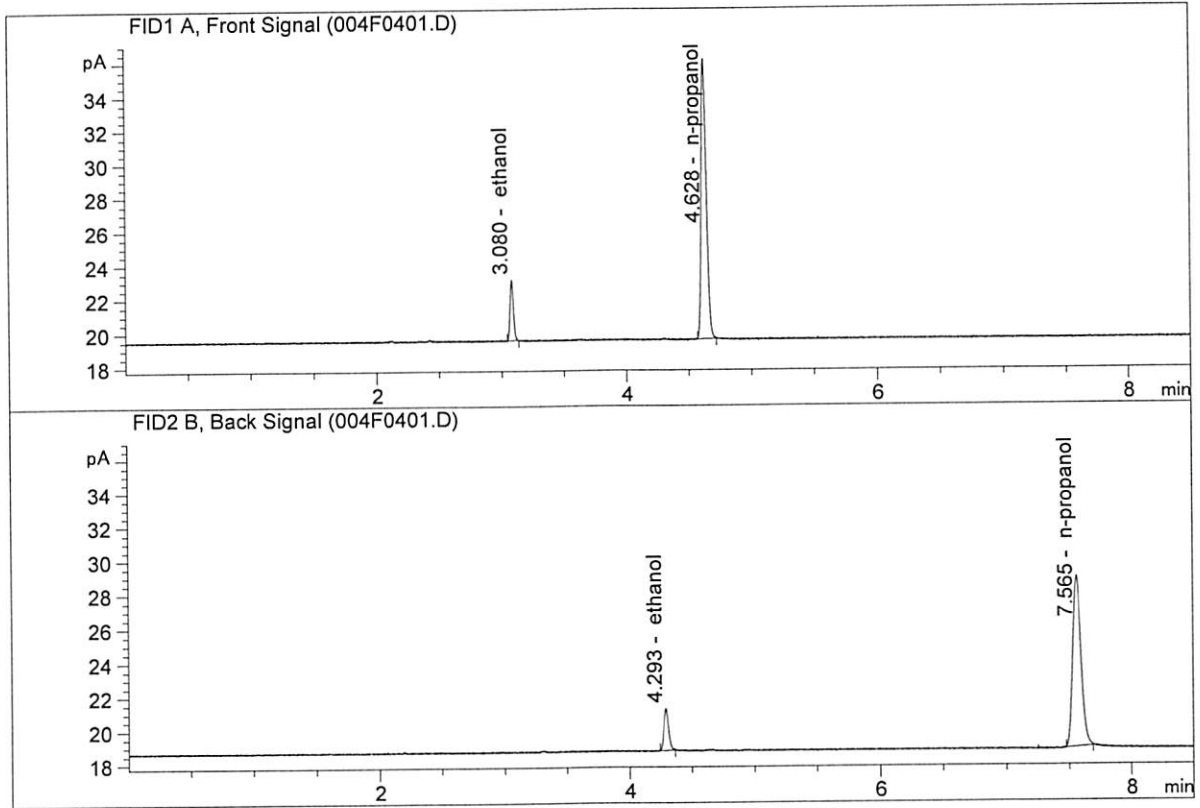

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	6.55964	0.0732	g/100cc
2.	Ethanol	Column 2:	6.68595	0.0745	g/100cc
3.	n-Propanol	Column 1:	47.17439	1.0000	g/100cc
4.	n-Propanol	Column 2:	48.18176	1.0000	g/100cc

MB

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: 0.08 FN09181807

Analysis Date(s): 18 Nov 2020

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Sample A-B Difference	Over-all Mean
Sample Results	0.0815	0.0824	0.0009	0.0819	0.0014	0.0826
(g/100cc)	0.0826	0.0840	0.0014	0.0833		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument information is stored centrally.

Refer to Instrument Method: Alcohol.m

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.082	0.077	0.087	0.005

Reported Result	
0.082	


Calibration and control data are stored centrally.

Revision: 2

Issue Date:

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.08 FN09181807-A
 Laboratory : Meridian
 Injection Date : Nov 18, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

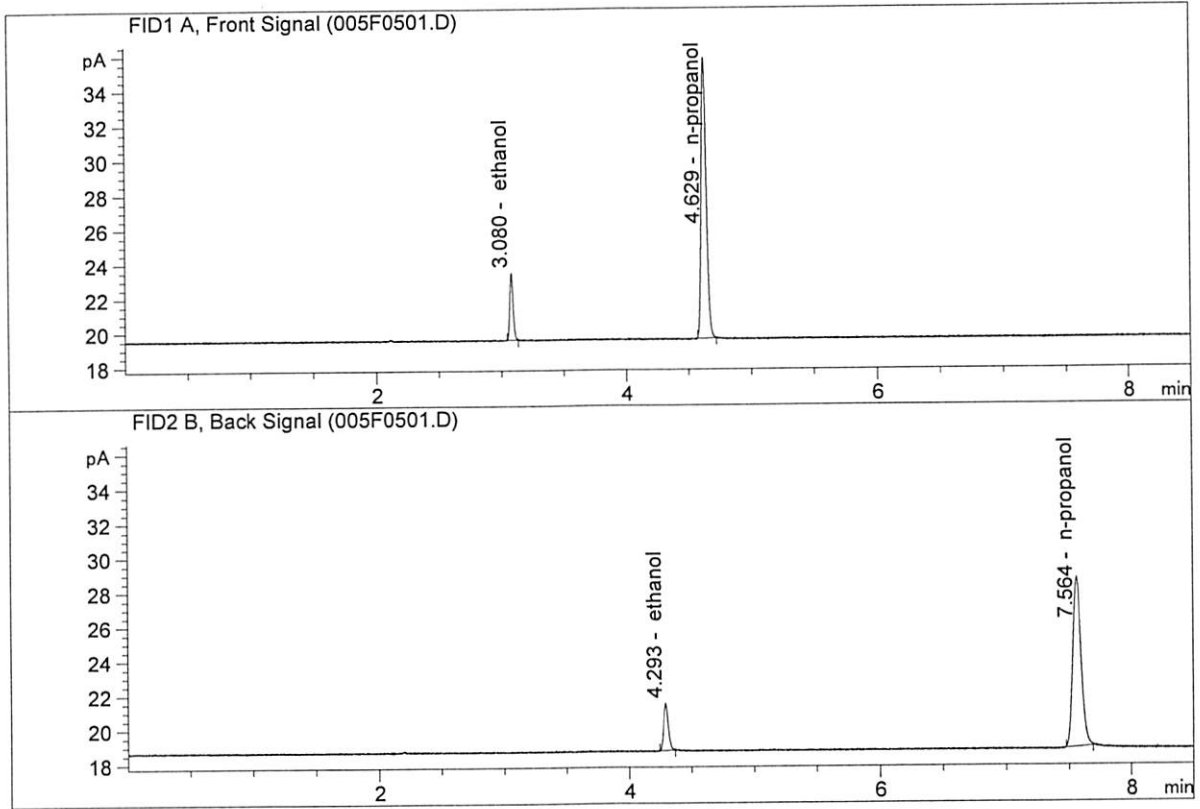


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.17682	0.0815	g/100cc
2.	Ethanol	Column 2:	7.28436	0.0824	g/100cc
3.	n-Propanol	Column 1:	46.23755	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.07112	1.0000	g/100cc

NS

ISP Forensic Services Blood Alcohol Report

Sample Name : 0.08 FN09181807-B
 Laboratory : Meridian
 Injection Date : Nov 18, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

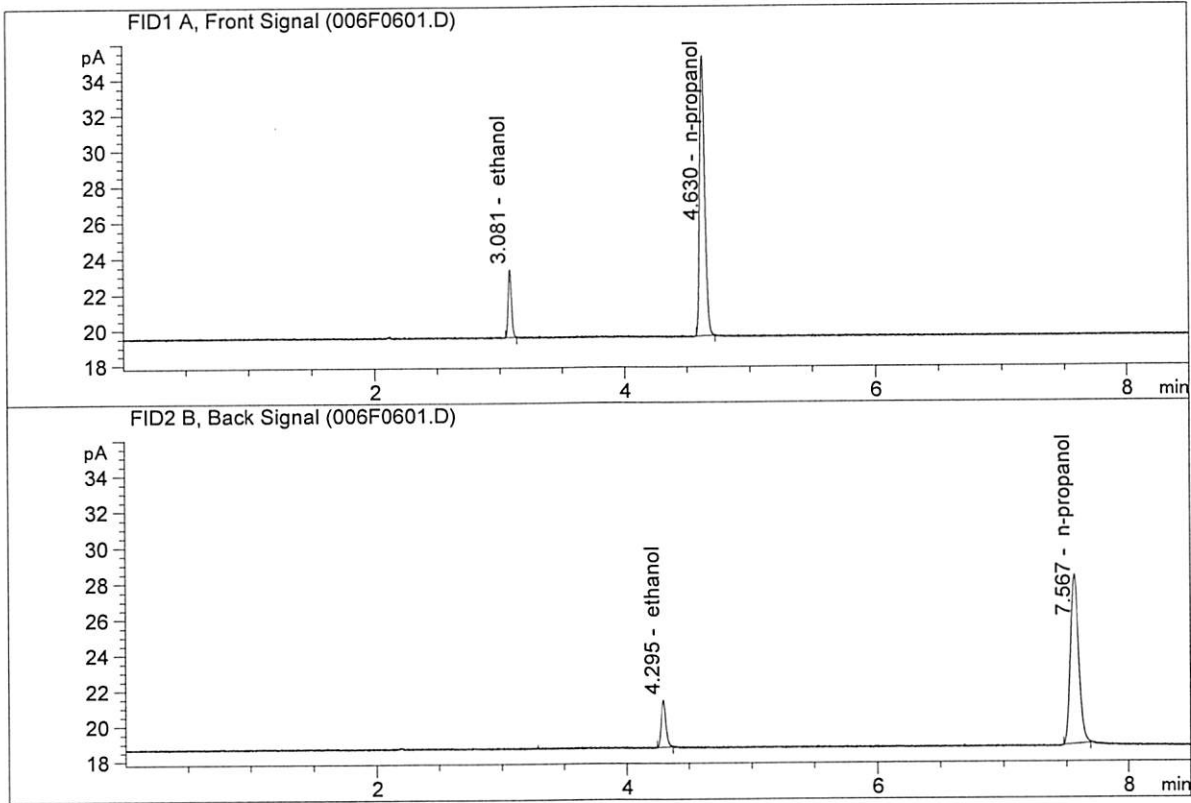

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	7.01127	0.0826	g/100cc
2.	Ethanol	Column 2:	7.15183	0.0840	g/100cc
3.	n-Propanol	Column 1:	44.52494	1.0000	g/100cc
4.	n-Propanol	Column 2:	45.26703	1.0000	g/100cc

NB

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC2-1

Analysis Date(s): 18 Nov 2020

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Sample A-B Difference	Over-all Mean
Sample Results	0.2036	0.2051	0.0015	0.2043	0.0000	0.2043
(g/100cc)	0.2041	0.2046	0.0005	0.2043		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument information is stored centrally.

Refer to Instrument Method: Alcohol.m

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.204	0.193	0.215	0.011

	Reported Result
	0.204

Calibration and control data are stored centrally.


NB

Revision: 2

Issue Date:

ISP Forensic Services Blood Alcohol Report

Sample Name : QC2-1-A
 Laboratory : Meridian
 Injection Date : Nov 18, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

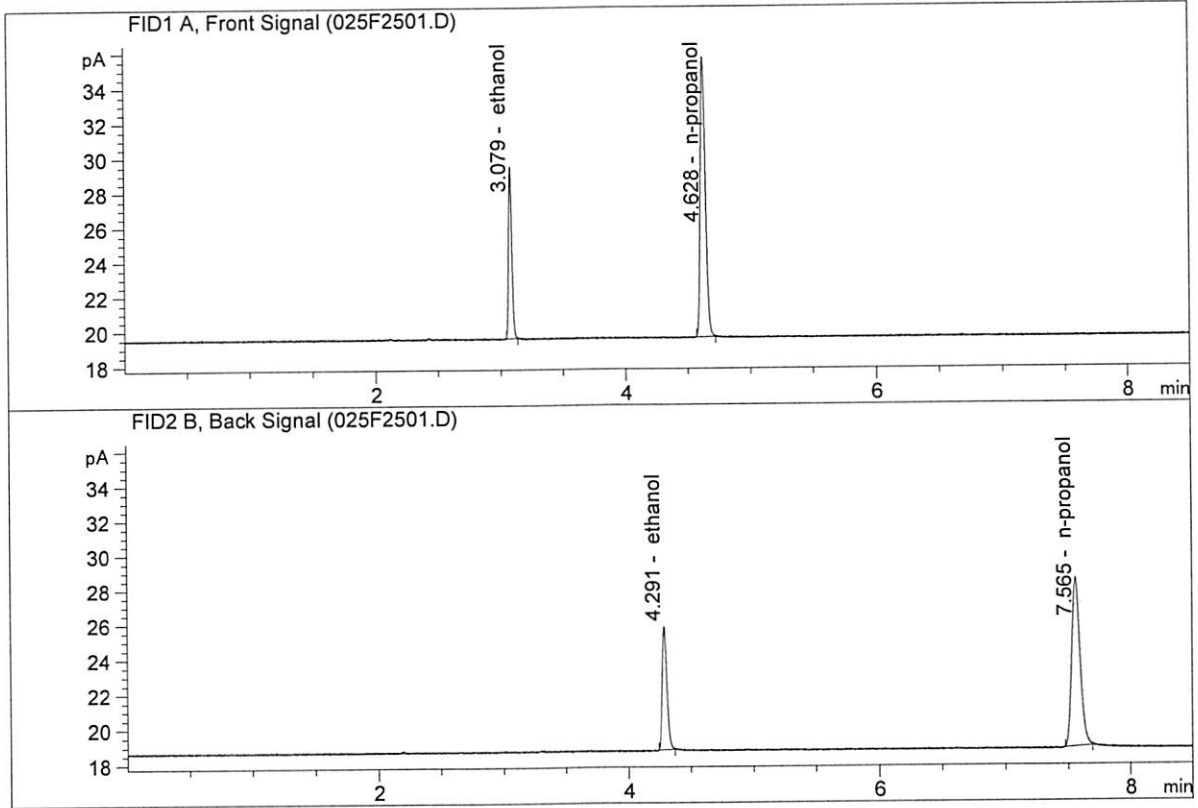


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	18.03858	0.2036	g/100cc
2.	Ethanol	Column 2:	18.73083	0.2051	g/100cc
3.	n-Propanol	Column 1:	45.77340	1.0000	g/100cc
4.	n-Propanol	Column 2:	46.44437	1.0000	g/100cc

NB

ISP Forensic Services Blood Alcohol Report

Sample Name : QC2-1-B
 Laboratory : Meridian
 Injection Date : Nov 18, 2020
 Method : ALCOHOL.M
 Acq. Instrument : CN11180014-CN11041167

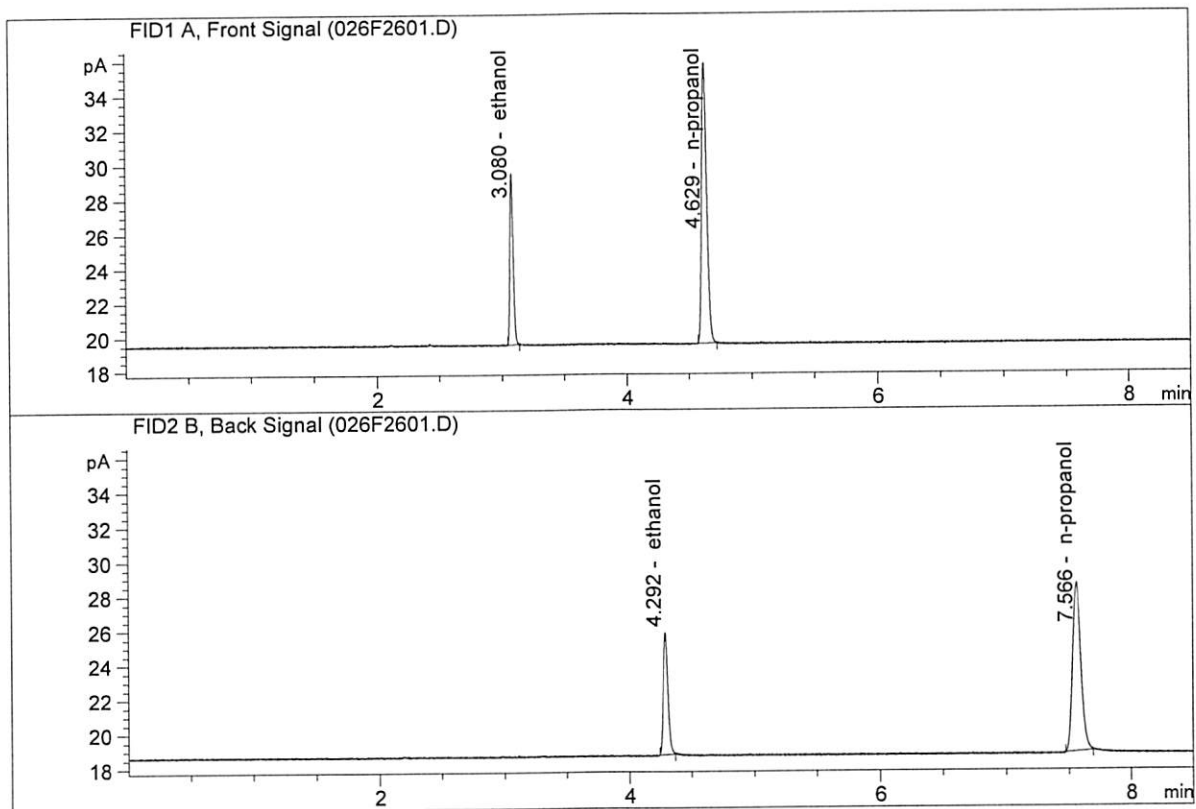

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	18.23616	0.2041	g/100cc
2.	Ethanol	Column 2:	18.85234	0.2046	g/100cc
3.	n-Propanol	Column 1:	46.14487	1.0000	g/100cc
4.	n-Propanol	Column 2:	46.84893	1.0000	g/100cc

NB

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC1-2

Analysis Date(s): 19 Nov 2020

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Sample A-B Difference	Over-all Mean
Sample Results	0.0750	0.0759	0.0009	0.0754	0.0005	0.0757
(g/100cc)	0.0755	0.0764	0.0009	0.0759		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument information is stored centrally.

Refer to Instrument Method: Alcohol.m

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.075	0.071	0.079	0.004

	Reported Result	
	0.075	


Calibration and control data are stored centrally.

Revision: 2

Issue Date:

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-2-A
 Laboratory : Meridian
 Injection Date : Nov 19, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

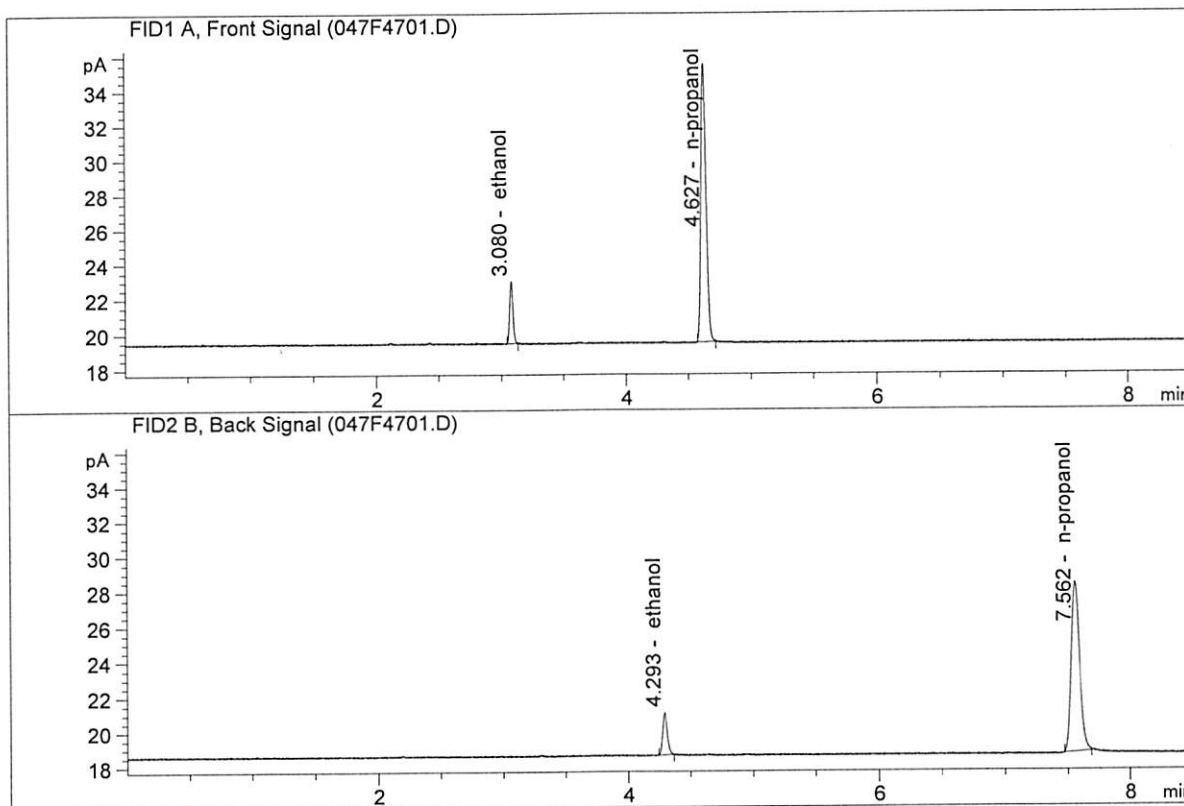


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	6.50794	0.0750	g/100cc
2.	Ethanol	Column 2:	6.55558	0.0759	g/100cc
3.	n-Propanol	Column 1:	45.62775	1.0000	g/100cc
4.	n-Propanol	Column 2:	46.34612	1.0000	g/100cc

NB

ISP Forensic Services Blood Alcohol Report

Sample Name : QC1-2-B
 Laboratory : Meridian
 Injection Date : Nov 19, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

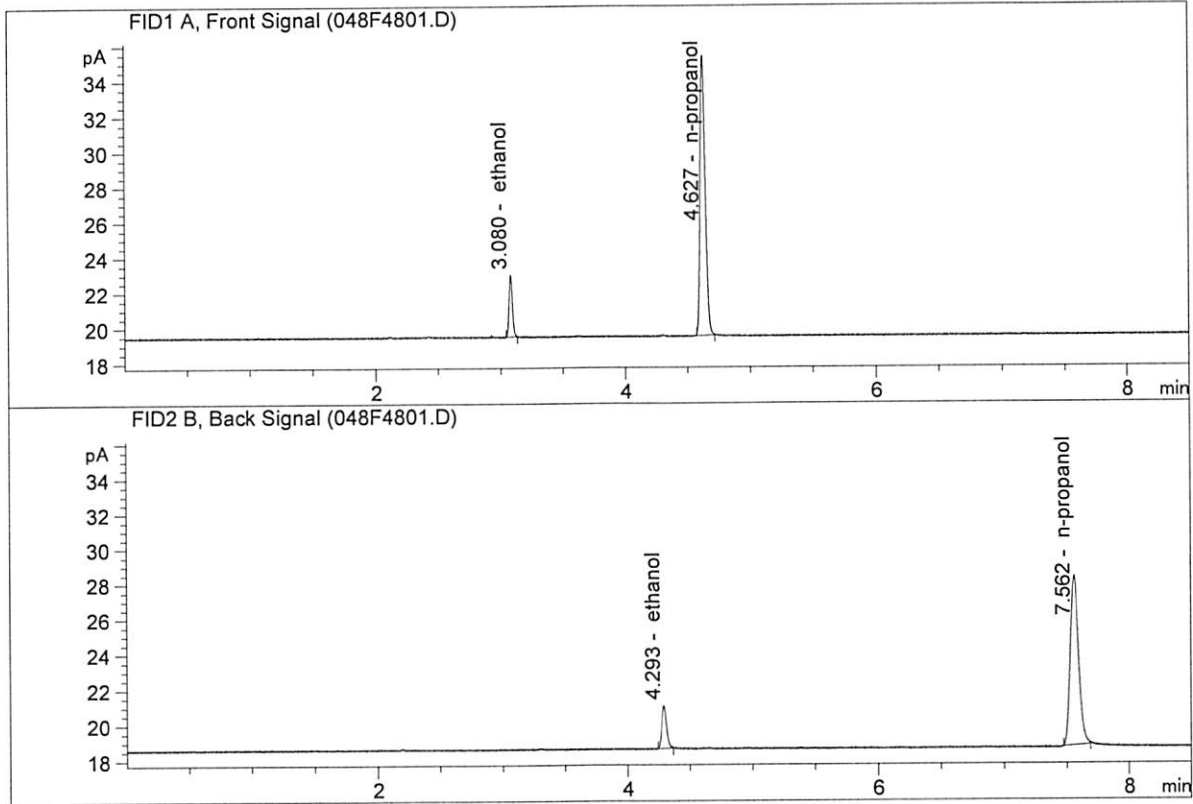

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	6.47950	0.0755	g/100cc
2.	Ethanol	Column 2:	6.53486	0.0764	g/100cc
3.	n-Propanol	Column 1:	45.16116	1.0000	g/100cc
4.	n-Propanol	Column 2:	45.81360	1.0000	g/100cc

MB

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No.: QC2-2

Analysis Date(s): 19 Nov 2020

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Sample A-B Difference	Over-all Mean
Sample Results	0.2062	0.2063	0.0001	0.2062	0.0018	0.2071
(g/100cc)	0.2077	0.2083	0.0006	0.2080		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument information is stored centrally.

Refer to Instrument Method: Alcohol.m

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%


Overall Mean (g/100cc)	Low	High	5% of Mean
0.207	0.196	0.218	0.011

	Reported Result
	0.207

Calibration and control data are stored centrally.

ISP Forensic Services Blood Alcohol Report

Sample Name : QC2-2-A
 Laboratory : Meridian
 Injection Date : Nov 19, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

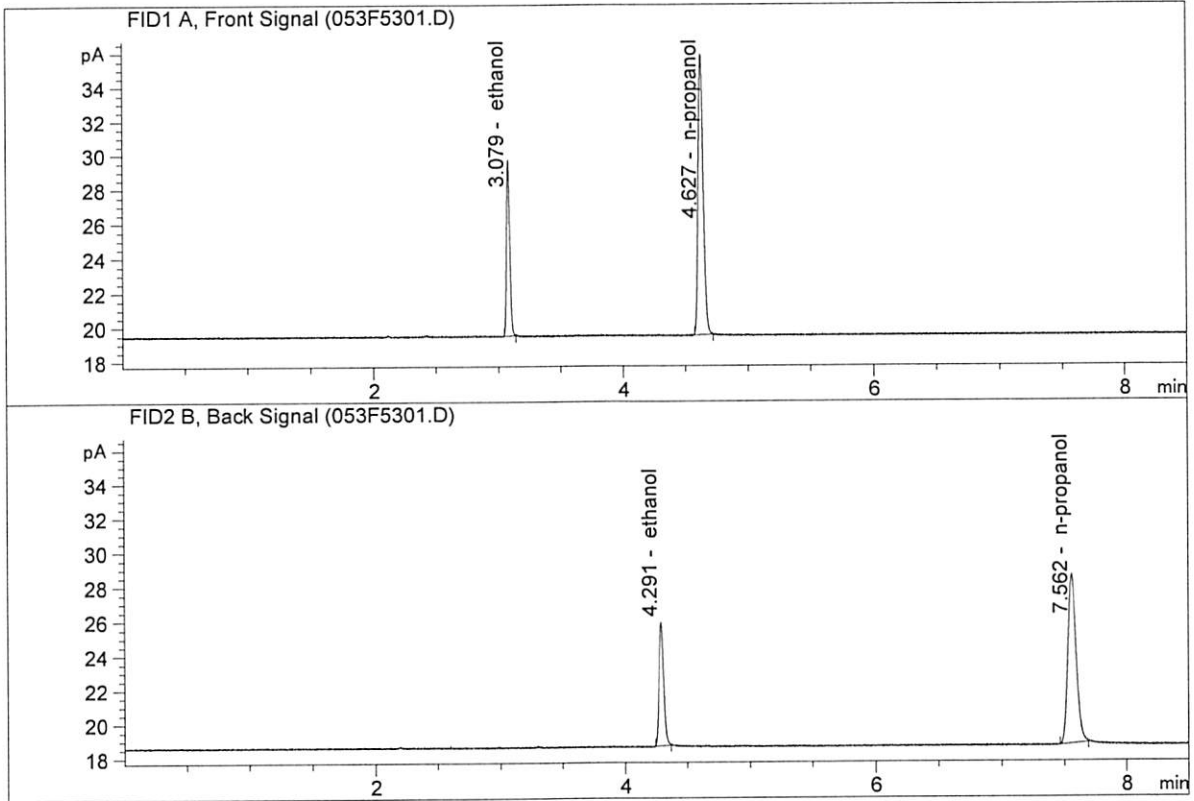


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	18.56322	0.2062	g/100cc
2.	Ethanol	Column 2:	19.21083	0.2063	g/100cc
3.	n-Propanol	Column 1:	46.50110	1.0000	g/100cc
4.	n-Propanol	Column 2:	47.32977	1.0000	g/100cc

MB

ISP Forensic Services Blood Alcohol Report

Sample Name : QC2-2-B
 Laboratory : Meridian
 Injection Date : Nov 19, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

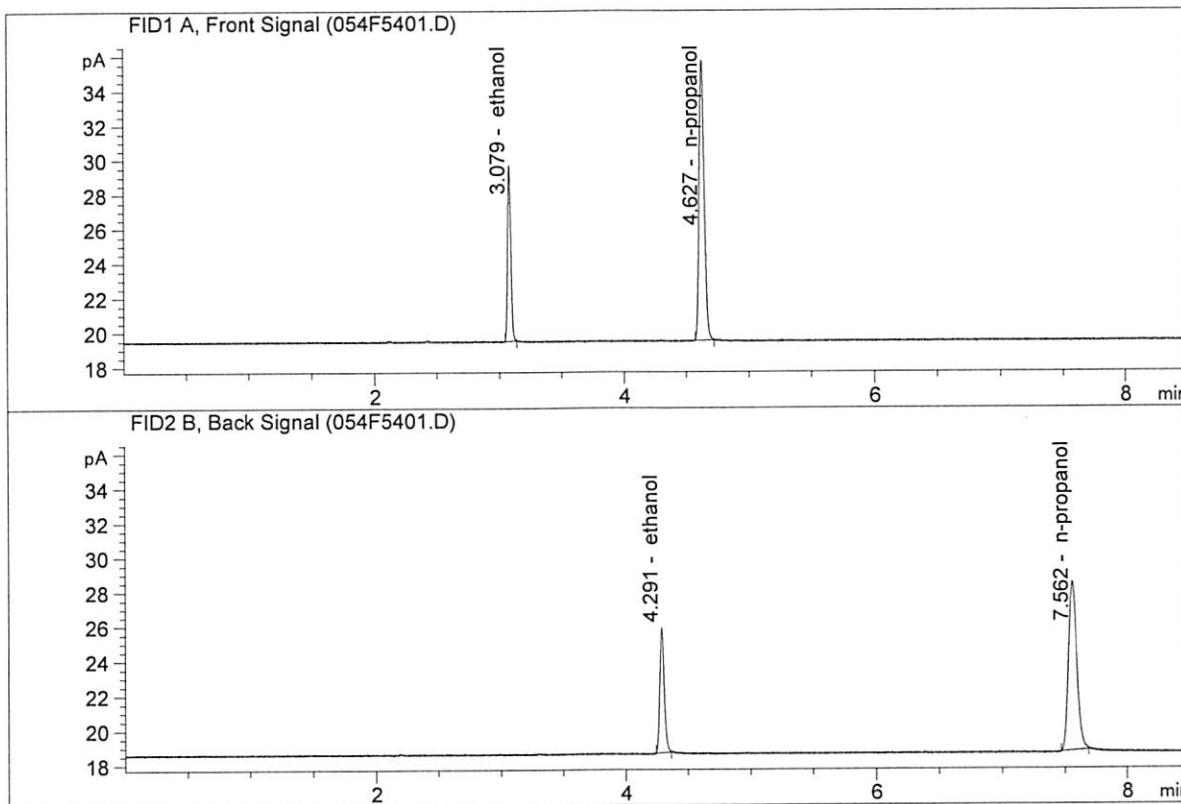


#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	18.53132	0.2077	g/100cc
2.	Ethanol	Column 2:	19.13923	0.2083	g/100cc
3.	n-Propanol	Column 1:	46.07932	1.0000	g/100cc
4.	n-Propanol	Column 2:	46.69530	1.0000	g/100cc

NB

ISP Forensic Services Blood Alcohol Report

Sample Name : INTERNAL STD BLK
 Laboratory : Meridian
 Injection Date : Nov 19, 2020
 Method : ALCOHOL.M
 Acq. Instrument: CN11180014-CN11041167

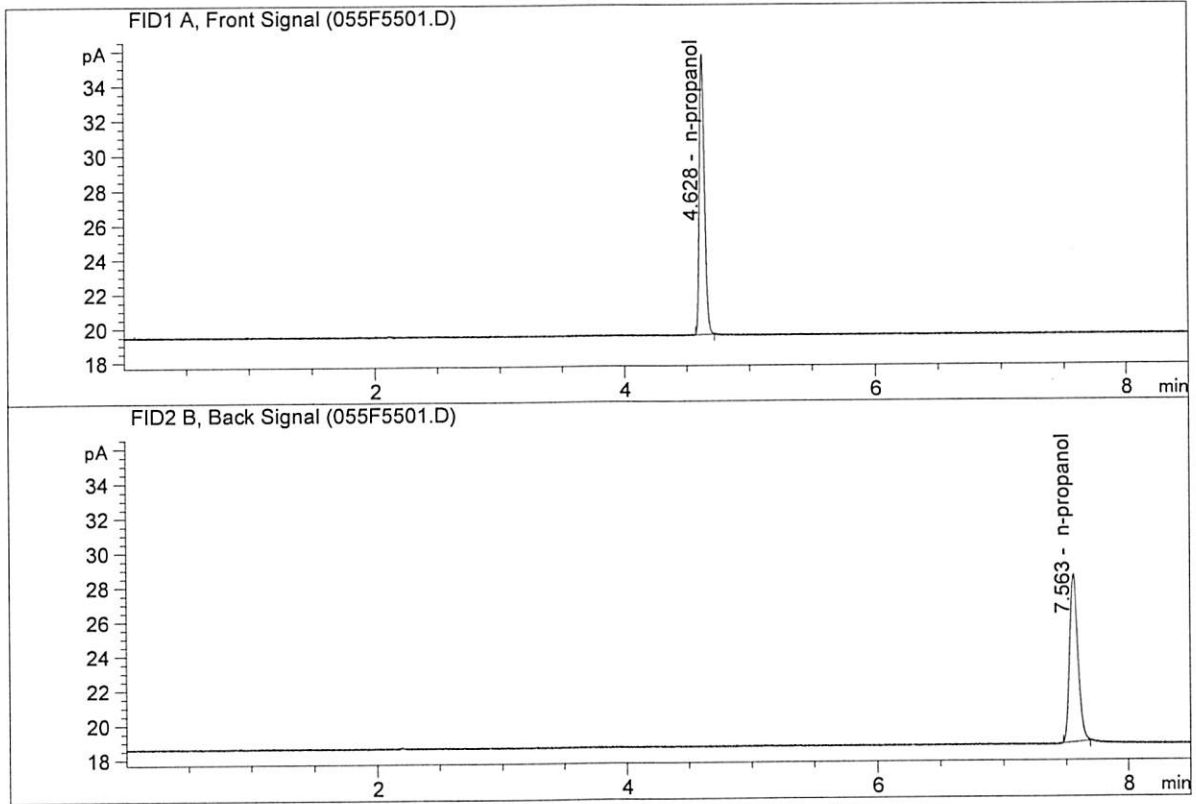

#	Compound	Column	Area	Amount	Units
1.	Ethanol	Column 1:	0.00000	0.0000	g/100cc
2.	Ethanol	Column 2:	0.00000	0.0000	g/100cc
3.	n-Propanol	Column 1:	45.93631	1.0000	g/100cc
4.	n-Propanol	Column 2:	46.58501	1.0000	g/100cc

NB

S a m p l e S u m m a r y

Sequence table: C:\Chem32\1\Data\11-18-20_SAMPLES\11-18-20_SAMPLES 2020-11-18 15-53-08\11-18-20_SAMPLES.S
 Data directory path: C:\Chem32\1\Data\11-18-20_SAMPLES\11-18-20_SAMPLES 2020-11-18 15-53-08\
 Logbook: C:\Chem32\1\Data\11-18-20_SAMPLES\11-18-20_SAMPLES 2020-11-18 15-53-08\11-18-20_SAMPLES.LOG
 Sequence start: 11/18/2020 4:07:52 PM
 Sequence Operator: SYSTEM
 Operator: SYSTEM
 Method file name: C:\Chem32\1\Data\11-18-20_SAMPLES\11-18-20_SAMPLES 2020-11-18 15-53-08\ALCOHOL.M

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #	# Cmp
1	1	1	INTERNAL STD BLK	-	1.0000	001F0101.D		2
2	2	1	MIX VOL FN007101	-	1.0000	002F0201.D		10
3	3	1	QC1-1-A	-	1.0000	003F0301.D		4
4	4	1	QC1-1-B	-	1.0000	004F0401.D		4
5	5	1	0.08 FN09181807-	-	1.0000	005F0501.D		4
6	6	1	0.08 FN09181807-	-	1.0000	006F0601.D		4
7	7	1	M2020-0952-16-A	-	1.0000	007F0701.D		4
8	8	1	M2020-0952-16-B	-	1.0000	008F0801.D		4
9	9	1	M2020-4564-1-A	-	1.0000	009F0901.D		4
10	10	1	M2020-4564-1-B	-	1.0000	010F1001.D		4
11	11	1	M2020-4565-1-A	-	1.0000	011F1101.D		4
12	12	1	M2020-4565-1-B	-	1.0000	012F1201.D		4
13	13	1	M2020-4577-2-A	-	1.0000	013F1301.D		2
14	14	1	M2020-4577-2-B	-	1.0000	014F1401.D		2
15	15	1	M2020-4585-1-A	-	1.0000	015F1501.D		4
16	16	1	M2020-4585-1-B	-	1.0000	016F1601.D		4
17	17	1	M2020-4586-1-A	-	1.0000	017F1701.D		4
18	18	1	M2020-4586-1-B	-	1.0000	018F1801.D		4
19	19	1	M2020-4594-1-A	-	1.0000	019F1901.D		4
20	20	1	M2020-4594-1-B	-	1.0000	020F2001.D		4
21	21	1	M2020-4614-1-A	-	1.0000	021F2101.D		4
22	22	1	M2020-4614-1-B	-	1.0000	022F2201.D		4
23	23	1	M2020-4617-1-A	-	1.0000	023F2301.D		4
24	24	1	M2020-4617-1-B	-	1.0000	024F2401.D		4
25	25	1	QC2-1-A	-	1.0000	025F2501.D		4
26	26	1	QC2-1-B	-	1.0000	026F2601.D		4
27	27	1	M2020-4626-1-A	-	1.0000	027F2701.D		2
28	28	1	M2020-4626-1-B	-	1.0000	028F2801.D		2
29	29	1	M2020-4630-2-A	-	1.0000	029F2901.D		2
30	30	1	M2020-4630-2-B	-	1.0000	030F3001.D		2
31	31	1	M2020-4667-1-A	-	1.0000	031F3101.D		4
32	32	1	M2020-4667-1-B	-	1.0000	032F3201.D		4
33	33	1	M2020-4668-1-A	-	1.0000	033F3301.D		4
34	34	1	M2020-4668-1-B	-	1.0000	034F3401.D		4
35	35	1	M2020-4670-1-A	-	1.0000	035F3501.D		2
36	36	1	M2020-4670-1-B	-	1.0000	036F3601.D		2
37	37	1	M2020-4671-1-A	-	1.0000	037F3701.D		4
38	38	1	M2020-4671-1-B	-	1.0000	038F3801.D		4
39	39	1	M2020-4672-1-A	-	1.0000	039F3901.D		4
40	40	1	M2020-4672-1-B	-	1.0000	040F4001.D		4
41	41	1	M2020-4673-1-A	-	1.0000	041F4101.D		4
42	42	1	M2020-4673-1-B	-	1.0000	042F4201.D		4
43	43	1	M2020-4680-1-A	-	1.0000	043F4301.D		4

NB

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #	# Cmp
44	44	1	M2020-4680-1-B	-	1.0000	044F4401.D		4
45	45	1	M2020-4687-1-A	-	1.0000	045F4501.D		4
46	46	1	M2020-4687-1-B	-	1.0000	046F4601.D		4
47	47	1	QC1-2-A	-	1.0000	047F4701.D		4
48	48	1	QC1-2-B	-	1.0000	048F4801.D		4
49	49	1	M2020-4688-1-A	-	1.0000	049F4901.D		4
50	50	1	M2020-4688-1-B	-	1.0000	050F5001.D		4
51	51	1	M2020-4689-1-A	-	1.0000	051F5101.D		4
52	52	1	M2020-4689-1-B	-	1.0000	052F5201.D		4
53	53	1	QC2-2-A	-	1.0000	053F5301.D		4
54	54	1	QC2-2-B	-	1.0000	054F5401.D		4
55	55	1	INTERNAL STD BLK	-	1.0000	055F5501.D		2

Method file name: C:\Chem32\1\Data\11-18-20_SAMPLES\11-18-20_SAMPLES 2020-11-18 15-53-08
 \SHUTDOWN.M

Run #	Location #	Inj #	Sample Name	Sample Amt [g/100cc]	Multip.* Dilution	File name	Cal #	# Cmp
56	56	1	EMPTY	-	1.0000	056F5601.D		0

MB