


Worklist: 5607


<u>LAB CASE</u>	<u>ITEM</u>	<u>ITEM TYPE</u>	<u>DESCRIPTION</u>
M2022-0460	1	BCK	Alcohol Analysis
M2022-0470	1	BCK	Alcohol Analysis
M2022-0476	2	BCK	Alcohol Analysis
M2022-0479	1	BCK	Alcohol Analysis
M2022-0502	1	BCK	Alcohol Analysis
M2022-0504	1	BCK	Alcohol Analysis
M2022-0505	1	BCK	Alcohol Analysis
M2022-0522	1	BCK	Alcohol Analysis
M2022-0544	1	BCK	Alcohol Analysis
M2022-0548	1	BCK	Alcohol Analysis
M2022-0549	1	BCK	Alcohol Analysis
M2022-0550	1	BCK	Alcohol Analysis
M2022-0566	1	BCK	Alcohol Analysis
M2022-0598	1	BCK	Alcohol Analysis
M2022-0599	1	BCK	Alcohol Analysis
M2022-0614	1	BCK	BATS Proficiency Test
M2022-0614	2	BCK	BATS Proficiency Test
M2022-0614	3	BCK	BATS Proficiency Test
M2022-0614	4	BCK	BATS Proficiency Test
M2022-0636	1	BCK	Alcohol Analysis
M2022-0637	1	BCK	Alcohol Analysis

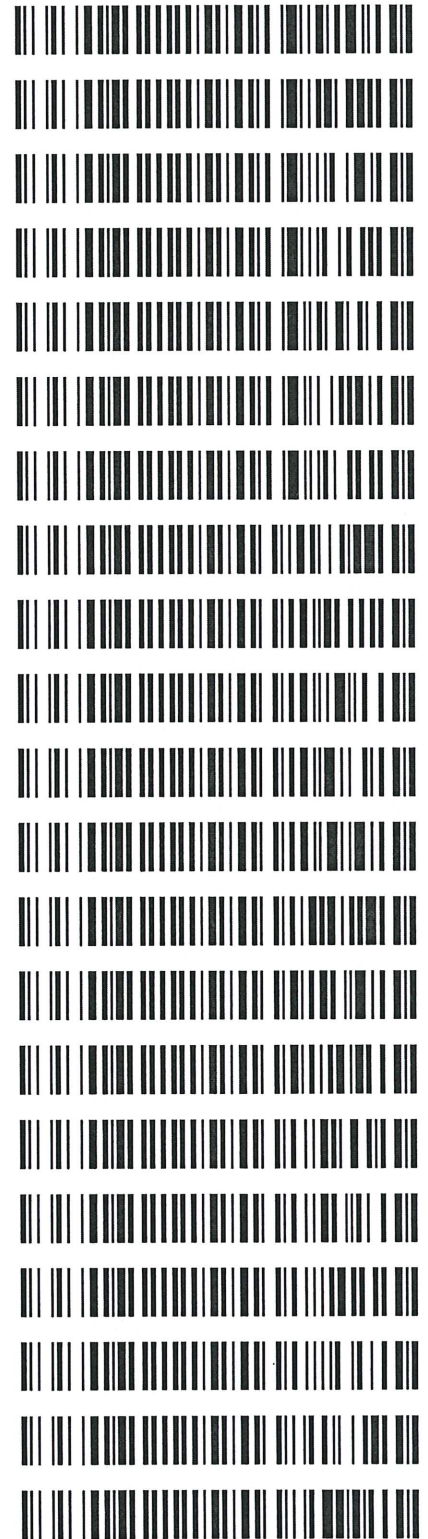

Handwritten signature or initials in blue ink.

Worklist: 5607

<u>LAB CASE</u>	<u>ITEM</u>	<u>ITEM TYPE</u>	<u>DESCRIPTION</u>
M2022-0638	1	BCK	Alcohol Analysis
M2022-0639	1	BCK	Alcohol Analysis
M2022-0640	1	BCK	Alcohol Analysis
M2022-0641	1	BCK	Alcohol Analysis
P2022-0333	1	BCK	Alcohol Analysis

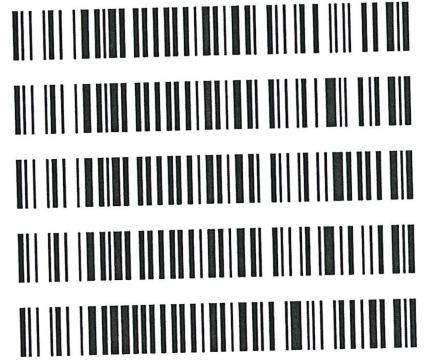

NB

Quantitative Analysis for Ethanol & Qualitative Analysis for Other Volatiles

Analytical Method(s): 1.0

Device: Hamilton MICROLAB Liquid Processor/Dilutor Serial Number: L600HC11378

Volatiles Quality Assurance Controls Run Date(s): 2/16/22 + 2/17/22 Qualitative

Calibration Date: 2/16/22; extraction: 2/16/22

Worklist #: 5607

Control level	Expiration	Lot #	Target Value	Acceptable Range	Overall Results
Level 1	Jul-23	1907006	0.0764	0.0688-0.0840	0.0737 g/100cc
					0.0779 g/100cc
Level 2	Jul-23	1907007	0.2170	0.1953-0.2387	0.2154 g/100cc
					0.2173 g/100cc
Multi-Component mixture: Curve Fit:					acceptable
		Exp: Jul-22	Lot # FN07101701		
		Column 1	0.99994	Column2	0.99997

Ethanol Calibration Reference Material

Calibrator level	Target Value	Acceptable Range	Column 1	Column 2	Precision	Mean
50	0.050	0.045 - 0.055	0.0513	0.0506	0.0007	0.0509
100	0.100	0.090 - 0.110	0.0997	0.1000	0.0003	0.0998
200	0.200	0.180 - 0.220	0.1996	0.2001	0.0005	0.1998
300	0.300	0.270 - 0.330	0.2978	0.2982	0.0004	0.298
400	0.400	0.360 - 0.440			0	#DIV/0!
500	0.500	0.450 - 0.550	0.5013	0.5009	0.0004	0.5011
Internal Standard	Average	(-) 20%		(+) 20%		
N-Propanol:	211244.8	168995.8		253493.7		

Aqueous Controls

Control level	Target Value	Acceptable Range	Overall Results
80	0.080	0.076 - 0.084	0.079 g/100cc

Handwritten initials: MB

Handwritten notes: MB 2/17/22 Qualitative

Internal Standard Monitoring Worksheet

Worklist #: 5607 Run Date(s): 2/16/22

Internal Standard Solution: Prep Date: 2/2/22 Exp Date: 8/2/22

Sample Name	Column 1 Value	Column 2 Value	Average
0.080A	196157	185157	190657
0.080B	194746	183753	189249.5
QC1-1A	197470	186218	191844
QC1-1B	203689	192175	197932
QC1-2A	226515	214004	220259.5
QC1-2B	222572	210382	216477
QC2-1A	224733	212013	218373
QC2-1B	223834	211364	217599
QC2-2A	231638	218325	224981.5
QC2-2B	252262	237888	245075
			#DIV/0!
			#DIV/0!
			#DIV/0!

Combined Average	(-)20%	(+)20%
211244.8	168995.8	253493.7



Revision: 4

Issue Date: 01/24/2022

Issuing Authority: Quality Manager

Idaho State Police
Forensic Services

Request for Departure from an Analytical Method or Quality Standard

Deviation Number (assigned by QM): BLA-22-01

Date of Request: 1/21/2022

Requestor/Discipline: Melissa (Nikka) Bradley/Blood Alcohol

Analytical Method/Quality Standard, Revision #: AM#1 Analysis for Volatiles by Headspace GC/ 4.3.9

Temporary or Permanent Deviation: Permanent

Scope of Deviation There is a noticeable increased drift of internal standard (n-propanol signals) from the calibrators, beginning of the run and towards the end of the sample run that is consistent in multiple batches of blood alcohol runs. Because all the samples that are analyzed are being compared to calibrators that are performed at the beginning of the run, the n-propanol signal of end samples tend to be outside or close to being outside of the +/- 20% of the mean value from the calibration curve used. Despite this drift the values of known control samples are within acceptable limits.

Deviation Request

4.3.9.1.1 The average values for the internal standard will be established by averaging the IS counts throughout the calibration curve samples.

Requesting that the internal standard monitoring average be changed to average the aqueous and matrix controls within the run.

4.3.9.1.1 The average values for the internal standard will be established by averaging the IS counts from the aqueous control and all matrix blood control samples.

Technical Justification for Analytical Method Deviations:

The designed purpose of the internal standard monitoring is to evaluate the quality of injection of each sample. There is a gradual increase of internal standard response from the beginning of the batch (calibrators and early samples) to the end that is inherent to the current instrument set up as shown in trends from previous batches in multiple laboratories. Attempts to pre-condition/warm up the instrument using by running a pre-batch sequence utilizing old calibrator/blank samples prior to running a new calibration curve did not appear to minimize this occurrence. Furthermore, it can be seen that the drifting trend is not due to the extraction procedure because some of the later batch samples were extracted prior to the samples that are injected during the run. It is worth noting that despite this

MB

trend, the values of the known control samples are still within the specified acceptable range. By utilizing known control n-propanol signals throughout the batch, any potential drift will be taken into account while still being able to monitor a possible mis-injection or partial injection throughout the batch/sequence.

This deviation will have an expiration date of July 1st, 2022.

Technical Review

Departure approved

Comments: Forms will be updated to reflect the new process concurrent with the deviation.

Departure Not Approved

Comments:

Approver:
Title: Discipline Lead

Date: 1/21/22

Quality Review

Quality Approver: Jason Crowe
Title: Quality Manager
Date: 01/24/2022



Calibration Table

Laboratory : MERIDIAN
 Instrument Name : GC-HS
 Instrument Serial # : C12595800409 / C12255750548


<<Data File>>

Method File :C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL_GCM
 Batch File :C:\LabSolutions\Data\220216\CALIBRATION\CALCURVE_TEMPLATE.gcb
 Date Acquired :2/16/2022 11:16:01 AM
 Date Created :2/16/2022 11:11:45 AM
 Date Modified :2/16/2022 11:19:04 AM



Name : Methanol
 Detector Name: FID1
 Function : $f(x)=0*x+0$
 R² value= 0
 FitType: Linear
 ZeroThrough: Not Through


#	Conc.	Area	Std. Conc.
---	-------	------	------------

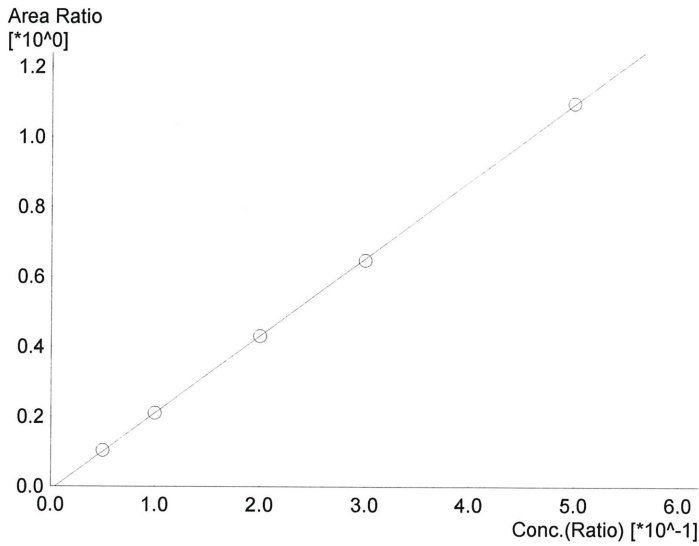

Name : Ethanol
 Detector Name: FID1
 Function : $f(x)=2.20630*x-0.0102597$
 R² value= 0.9999369
 FitType: Linear
 ZeroThrough: Not Through


#	Conc.	Area	Std. Conc.
1	0.050	19673	0.0513
2	0.100	40476	0.0997
3	0.200	81184	0.1996
4	0.300	122967	0.2978
5	0.500	219373	0.5013

NB

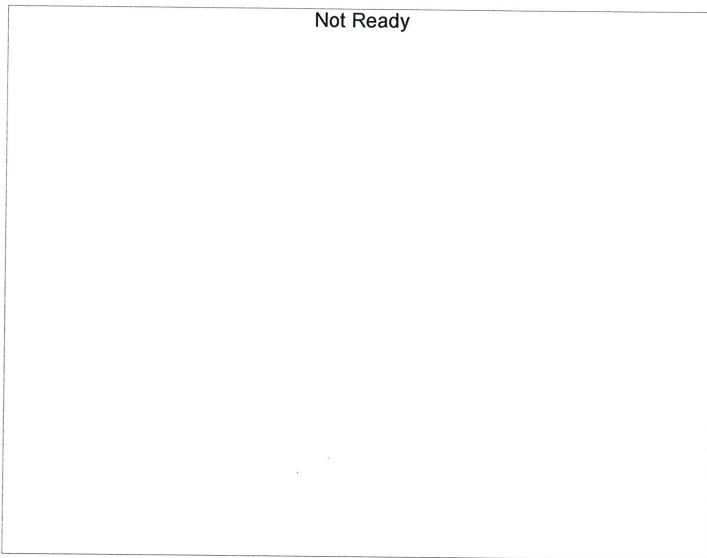


Name : Isopropyl Alcohol
Detector Name: FID1
Function : $f(x)=0*x+0$
R² value= 0
FitType: Linear
ZeroThrough: Not Through

#	Conc.	Area	Std. Conc.
---	-------	------	------------

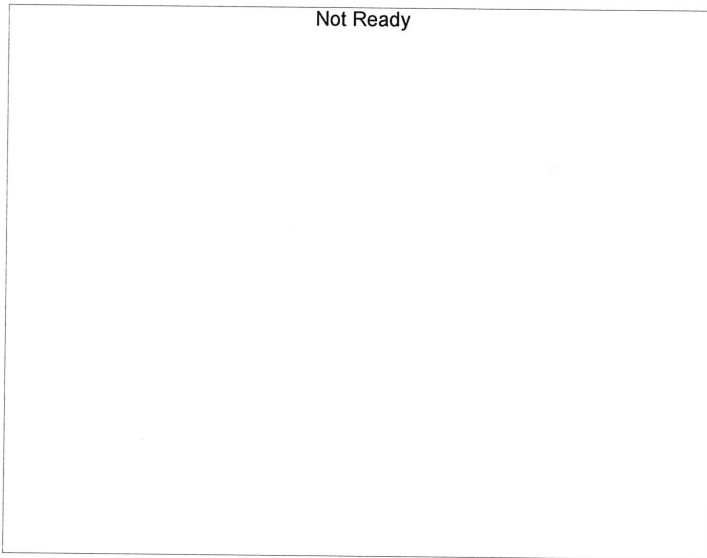


Name : Acetone
Detector Name: FID1
Function : $f(x)=0*x+0$
R² value= 0
FitType: Linear
ZeroThrough: Not Through

#	Conc.	Area	Std. Conc.
---	-------	------	------------

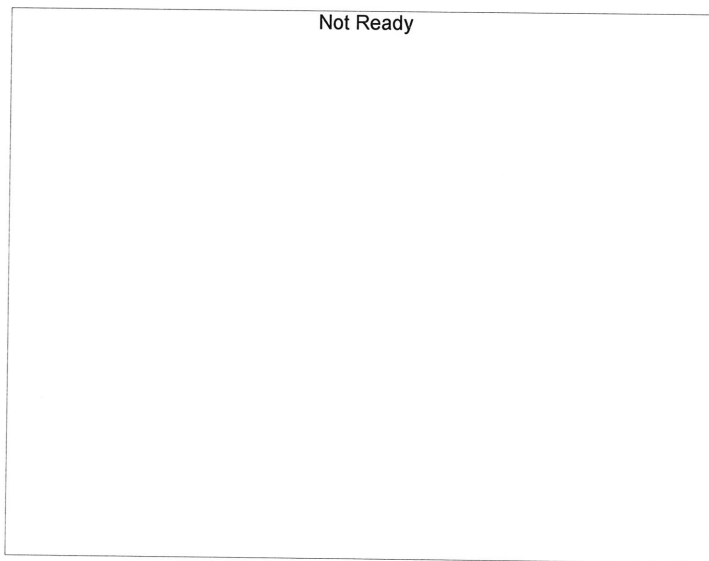


Name : Fluor. Hydrocarbon(s)
Detector Name: FID1
Function : $f(x)=0*x+0$
R² value= 0
FitType: Linear
ZeroThrough: Not Through

#	Conc.	Area	Std. Conc.
---	-------	------	------------

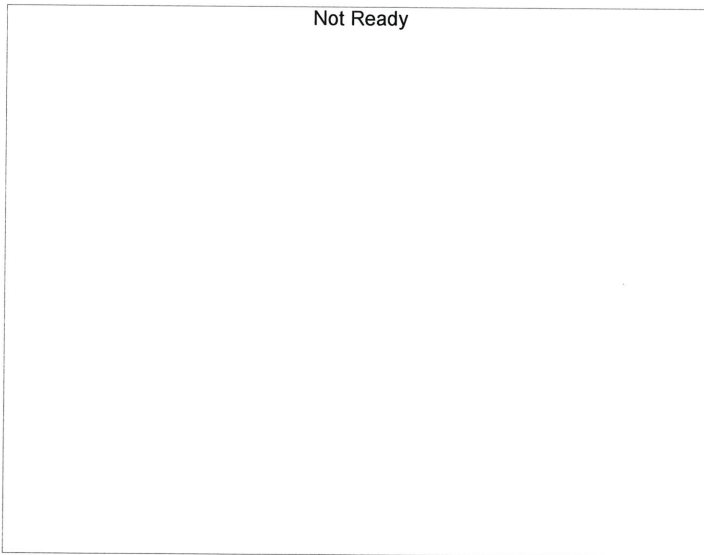


Name : Methanol
 Detector Name: FID2
 Function : $f(x)=0*x+0$
 R² value= 0
 FitType: Linear
 ZeroThrough: Not Through

#	Conc.	Area	Std. Conc.
---	-------	------	------------

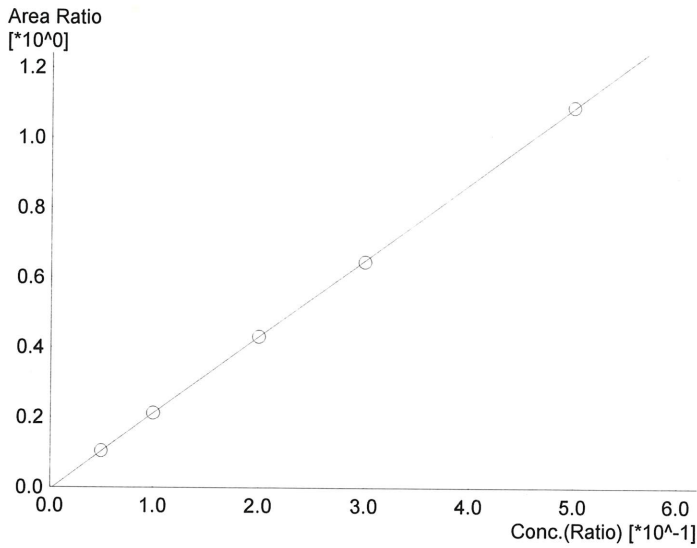

Name : Ethanol
 Detector Name: FID2
 Function : $f(x)=2.18326*x-0.00645134$
 R² value= 0.9999674
 FitType: Linear
 ZeroThrough: Not Through


#	Conc.	Area	Std. Conc.
1	0.050	18802	0.0506
2	0.100	38521	0.1000
3	0.200	76571	0.2001
4	0.300	115471	0.2982
5	0.500	204308	0.5009

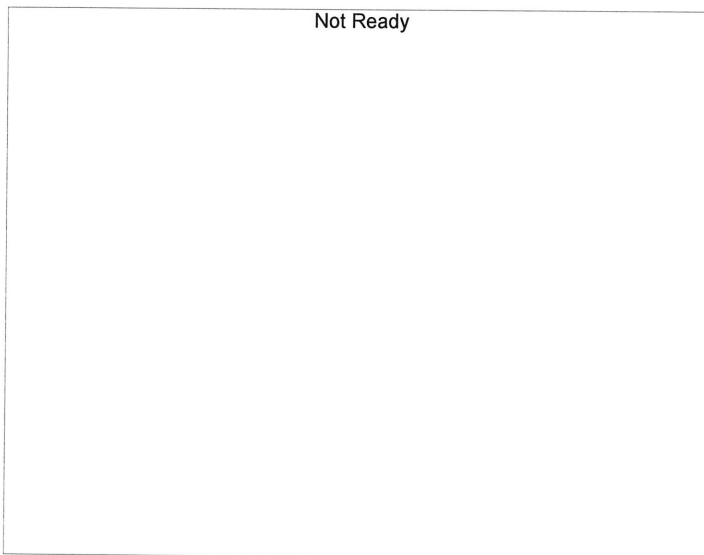

Name : Acetone
 Detector Name: FID2
 Function : $f(x)=0*x+0$
 R² value= 0
 FitType: Linear
 ZeroThrough: Not Through

#	Conc.	Area	Std. Conc.
---	-------	------	------------

NB

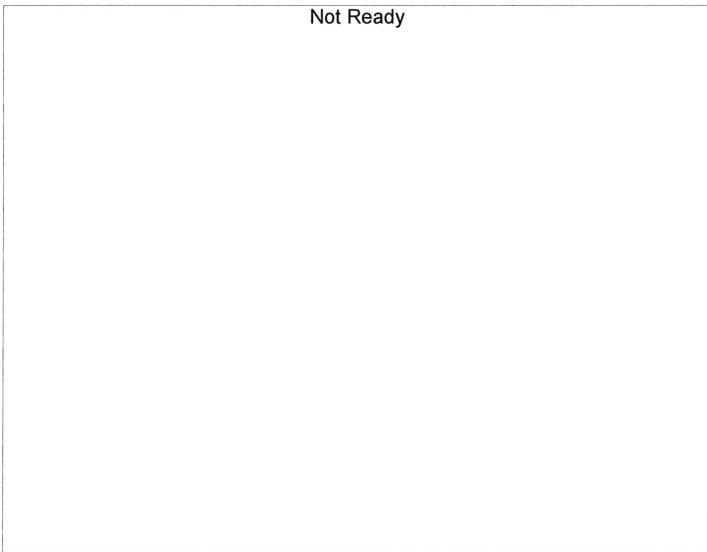

Name : Isopropyl Alcohol
Detector Name: FID2
Function : $f(x)=0*x+0$
R² value= 0
FitType: Linear
ZeroThrough: Not Through

#	Conc.	Area	Std. Conc.
---	-------	------	------------





Name : Fluor. Hydrocarbon(s)
Detector Name: FID2
Function : $f(x)=0*x+0$
R² value= 0
FitType: Linear
ZeroThrough: Not Through

#	Conc.	Area	Std. Conc.
---	-------	------	------------

NB

Sample Name : 0.050
 Laboratory : Meridian
 Injection Date : 2/16/2022 10:45:01 AM
 Vial # : 1
 Method Filename : C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
 Instrument #GC/HS : C12255750548 / C12595800409

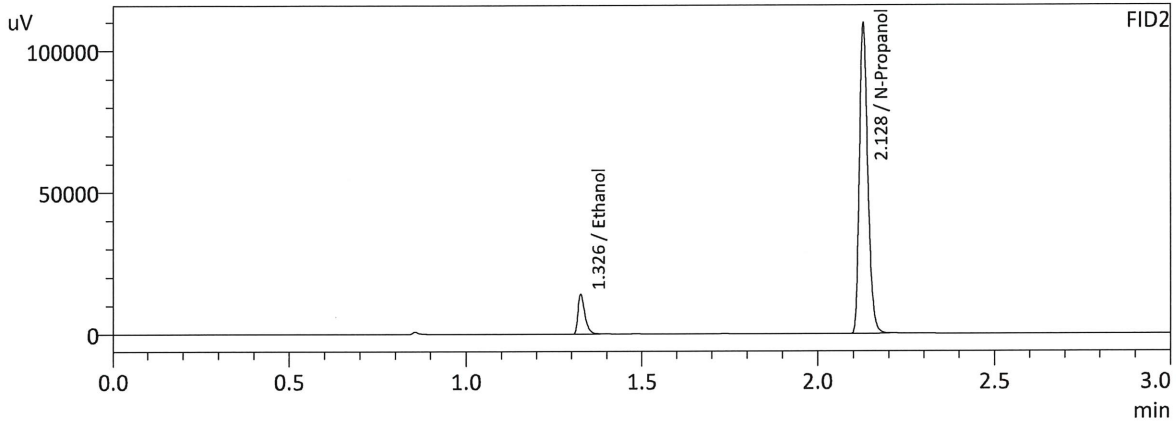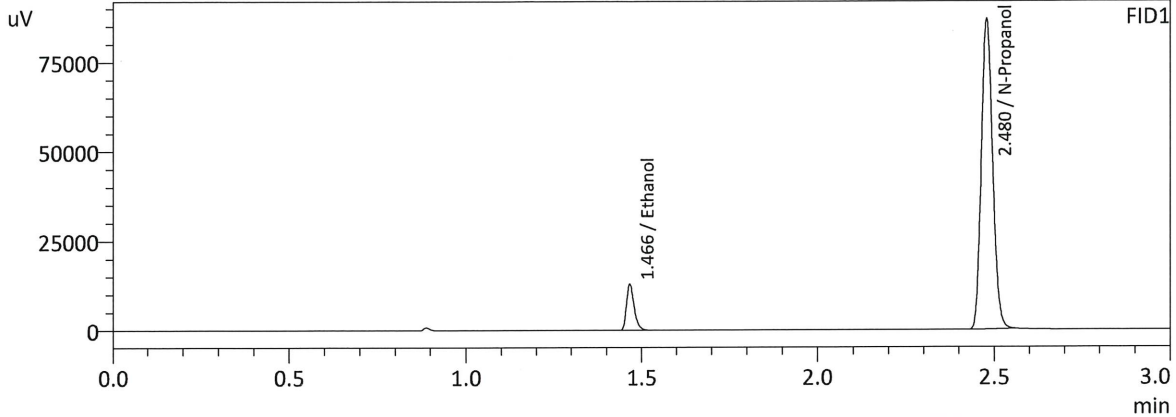

FID1



Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.0513	19673	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	191026	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.0506	18802	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	180488	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

NB

Sample Name : 0.100
 Laboratory : Meridian
 Injection Date : 2/16/2022 10:52:23 AM
 Vial # : 2
 Method Filename : C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
 Instrument #GC/HS : C12255750548 / C12595800409

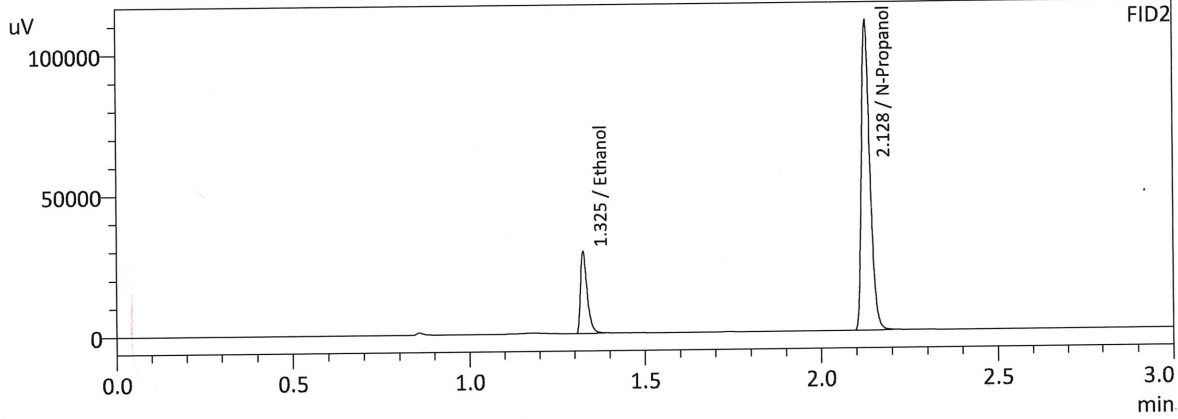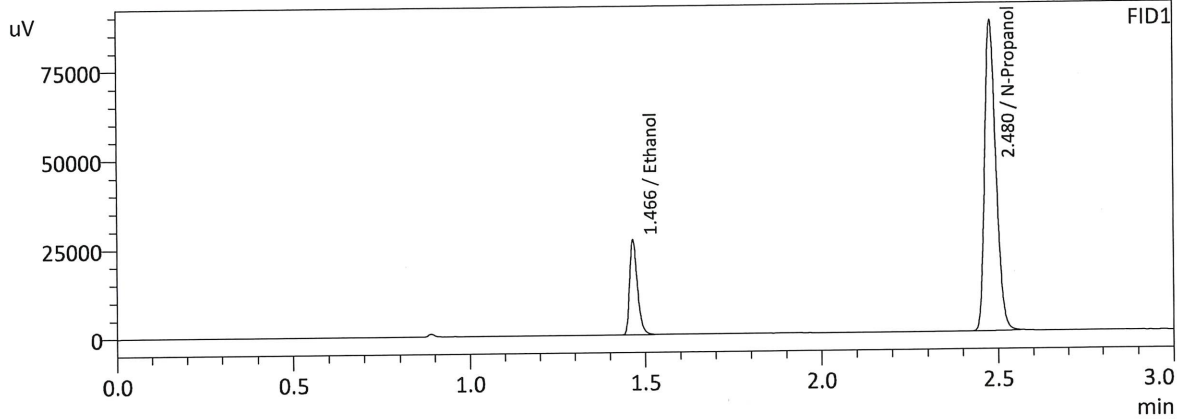

FID1



Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.0997	40476	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	192812	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.1000	38521	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	181805	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

NB

Sample Name : 0.200
 Laboratory : Meridian
 Injection Date : 2/16/2022 10:59:40 AM
 Vial # : 3
 Method Filename : C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
 Instrument #GC/HS : C12255750548 / C12595800409

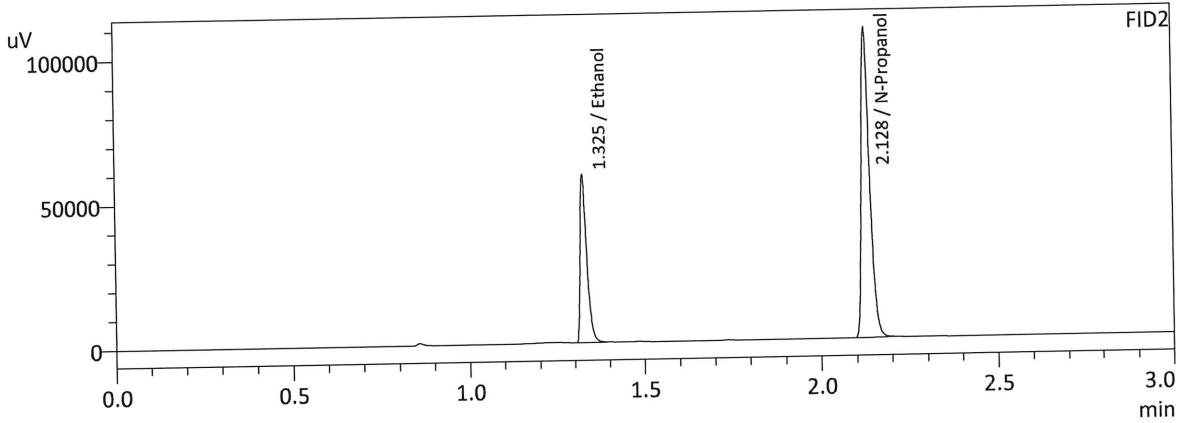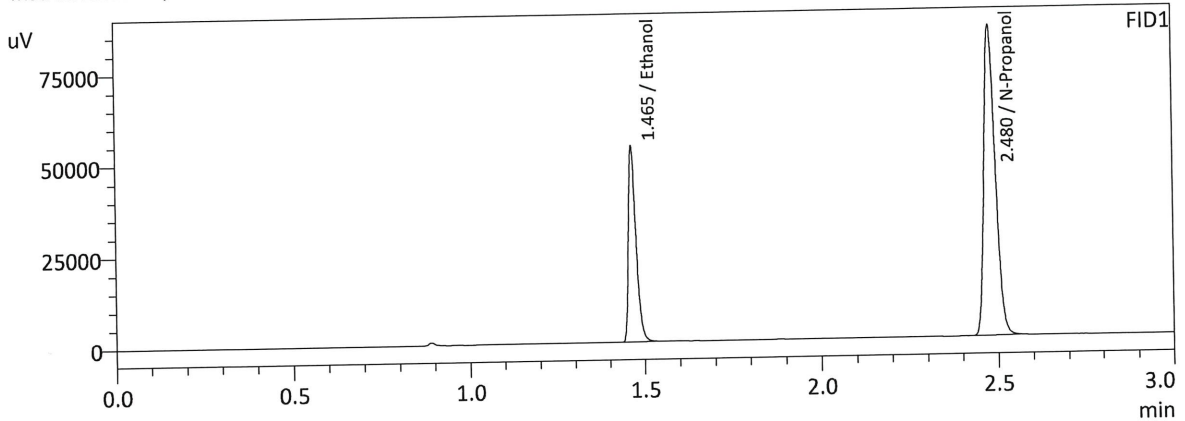

FID1



Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.1996	81184	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	188662	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.2001	76571	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	177877	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

NB

Sample Name : 0.300
 Laboratory : Meridian
 Injection Date : 2/16/2022 11:08:36 AM
 Vial # : 4
 Method Filename : C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
 Instrument #GC/HS : C12255750548 / C12595800409

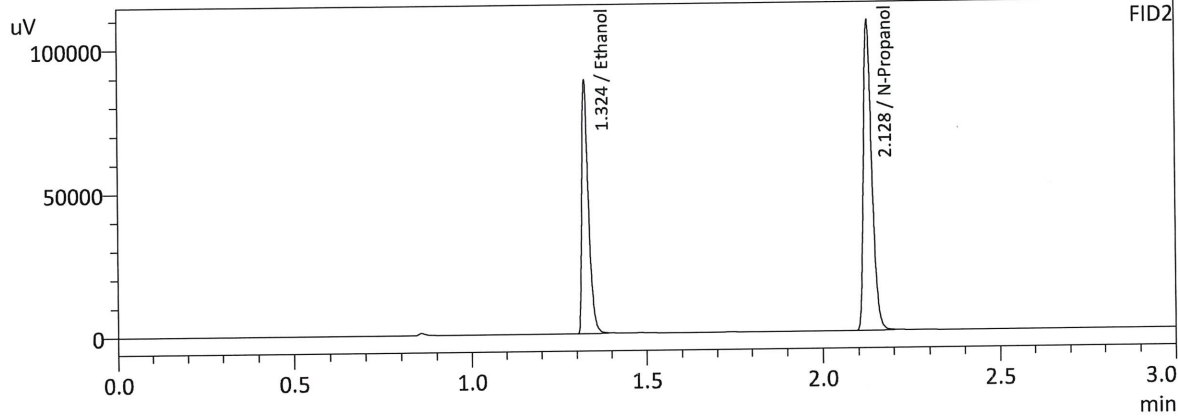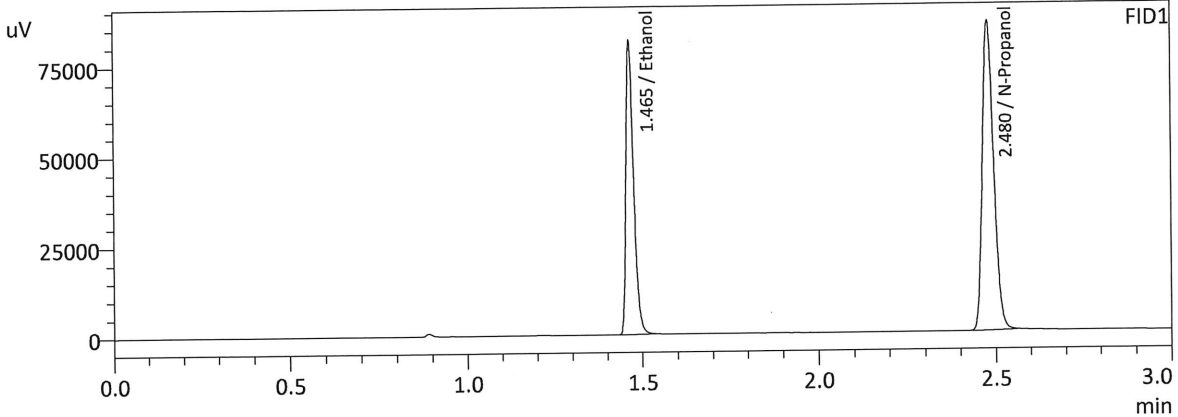

FID1



Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.2978	122967	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	190070	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.2982	115471	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	179077	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

NB

Sample Name : 0.500
 Laboratory : Meridian
 Injection Date : 2/16/2022 11:16:01 AM
 Vial # : 5
 Method Filename : C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
 Instrument #GC/HS : C12255750548 / C12595800409

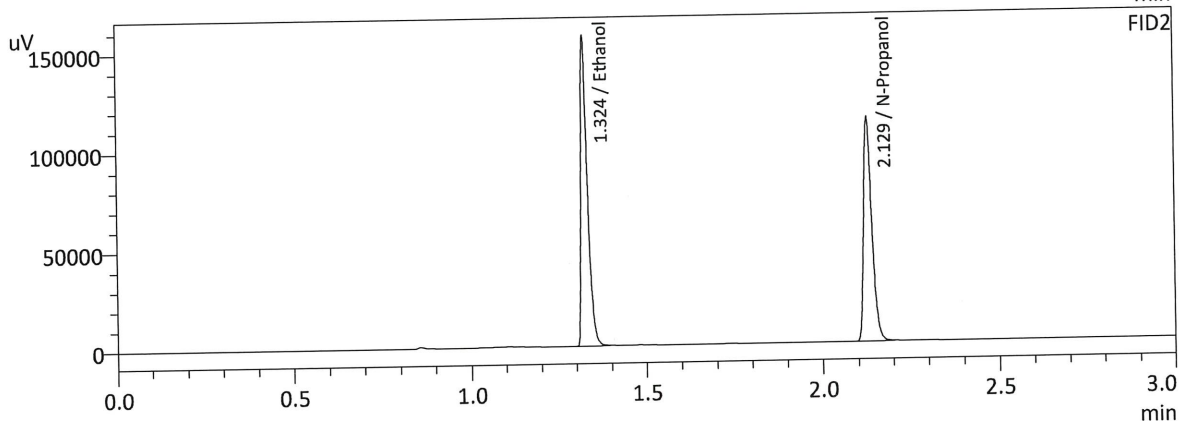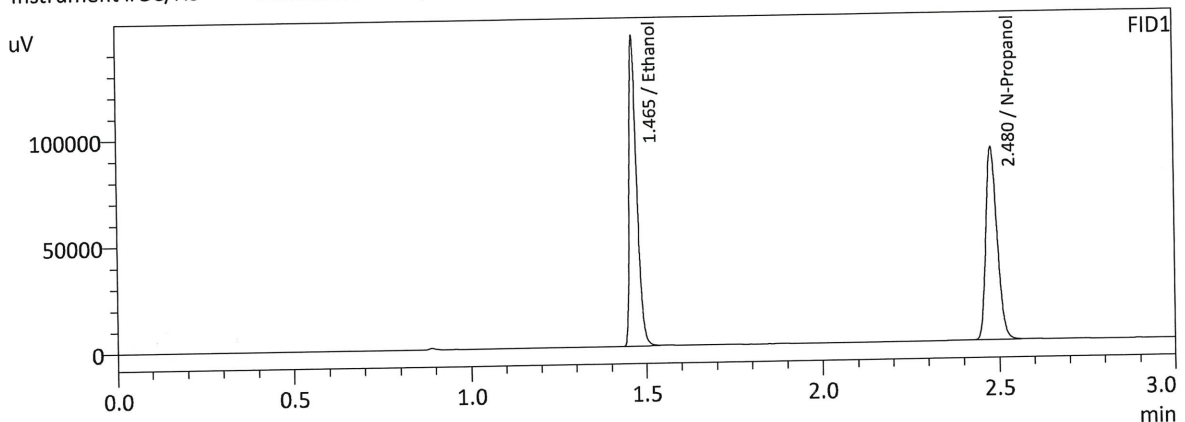

FID1



Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.5013	219373	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	200201	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.5009	204308	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	187929	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

NB

Sample Name : INT STD BLK
 Laboratory : Meridian
 Injection Date : 2/16/2022 11:24:35 AM
 Vial # : 6
 Method Filename : C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
 Instrument #GC/HS : C12255750548 / C12595800409

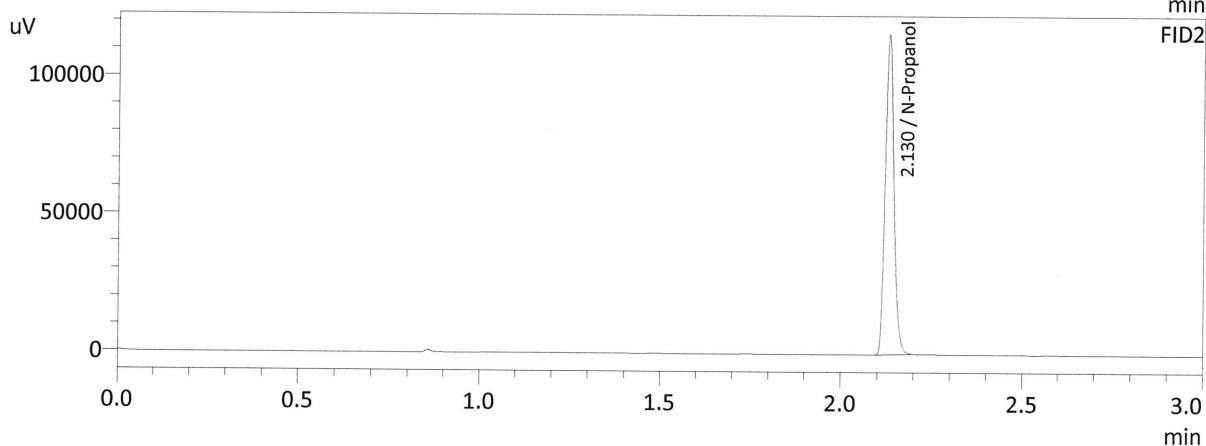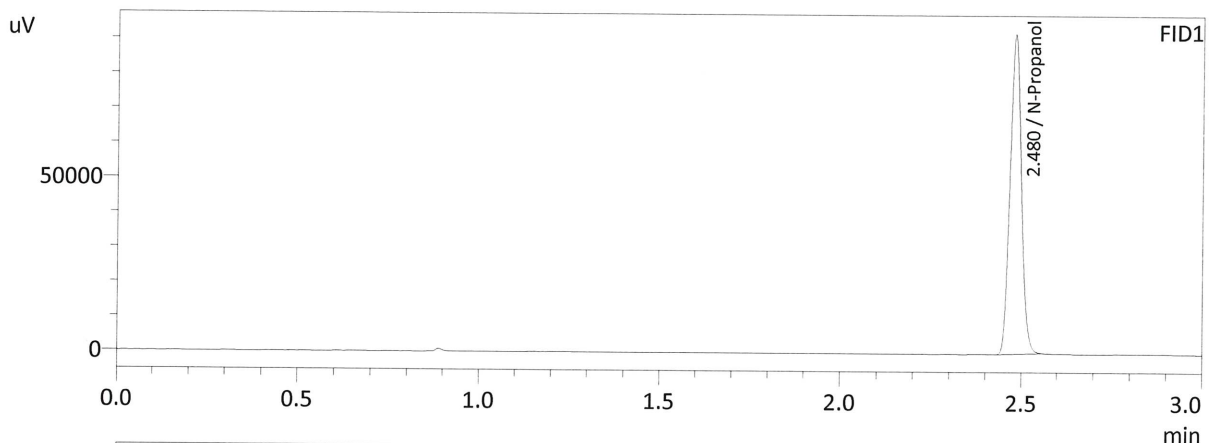

FID1

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	203319	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	--	--	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	192158	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

NB



Meridian Blood Alcohol Analysis Batch Table

Shimadzu GC-2030 Serial #C12255750548
Shimadzu HS-20 Serial #C12595800409
Lab Solutions Software Ver. 5.99
Copyright (C) 2008-2020 Shimadzu Corporation

Vial#	Sample Name	Sample Type	Level#	Method File
1	0.050	1:Standard:(I)	1	ALCOHOL.GCM
2	0.100	1:Standard	2	ALCOHOL.GCM
3	0.200	1:Standard	3	ALCOHOL.GCM
4	0.300	1:Standard	4	ALCOHOL.GCM
5	0.500	1:Standard	5	ALCOHOL.GCM
6	INT STD BLK	0:Unknown	0	ALCOHOL.GCM



Sample Name : INT STD BLK 1
 Laboratory : Meridian
 Injection Date : 2/16/2022 12:40:47 PM
 Vial # : 1
 Method Filename : C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
 Instrument #GC/HS : C12255750548 / C12595800409

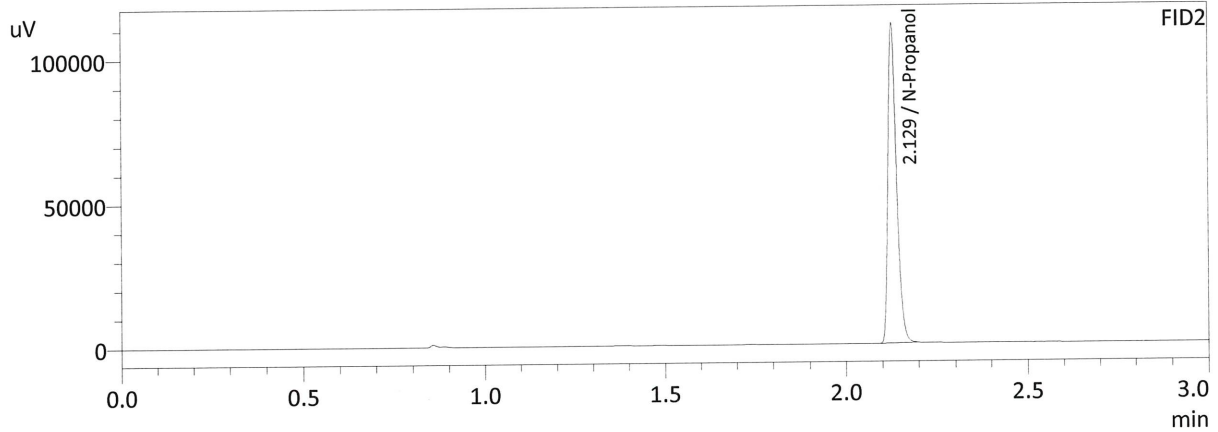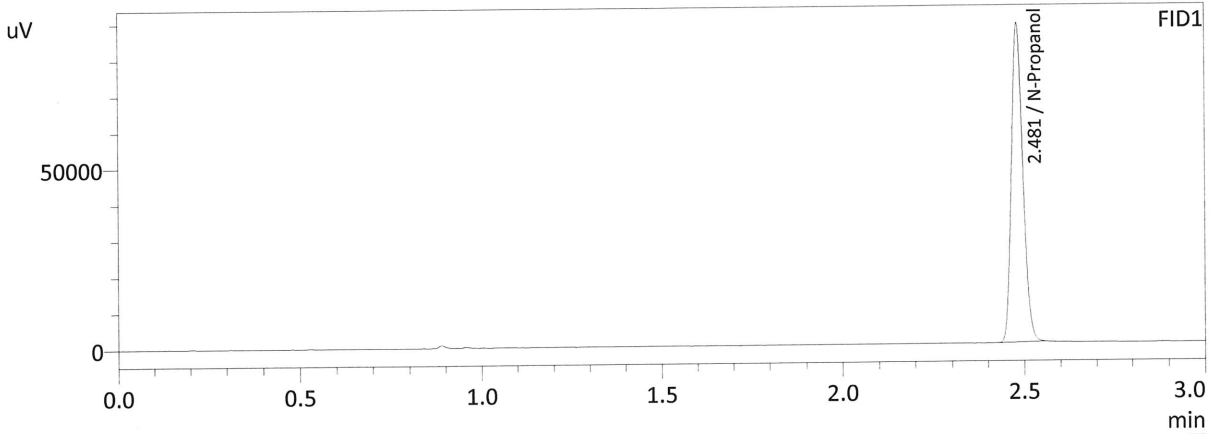

FID1



Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	194764	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	--	--	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	184138	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

LB

Sample Name : MIXED VOLATILES FN 07101701
 Laboratory : Meridian
 Injection Date : 2/16/2022 12:48:08 PM
 Vial # : 2
 Method Filename : C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
 Instrument #GC/HS : C12255750548 / C12595800409

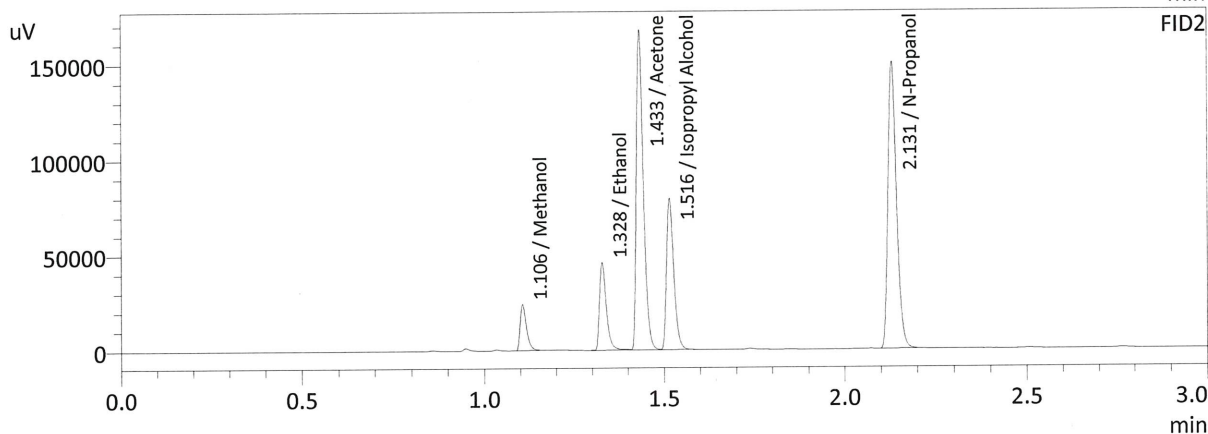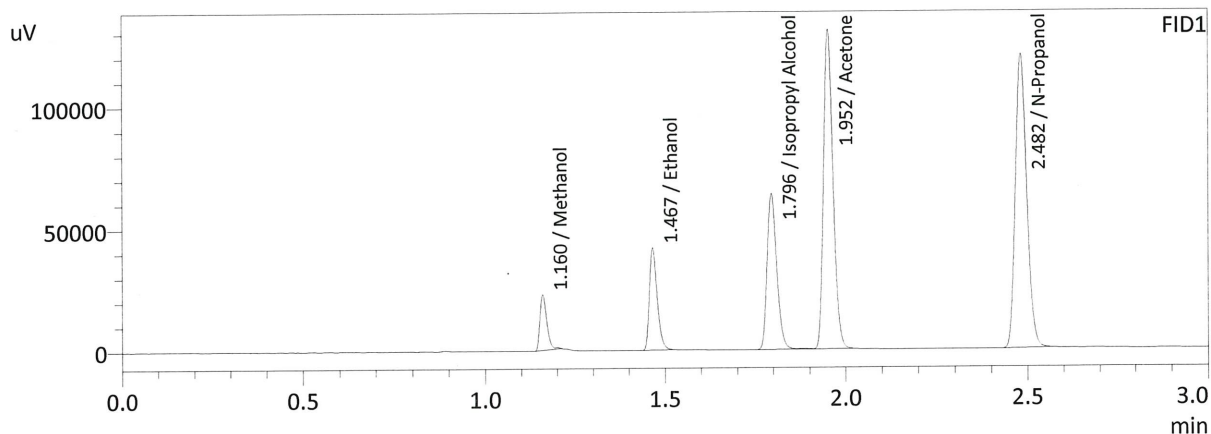

FID1

Name	Conc.	Area	Unit
Methanol	0.0000	30440	g/100cc
Ethanol	0.1140	63917	g/100cc
Isopropyl Alcohol	0.0000	117872	g/100cc
Acetone	0.0000	241296	g/100cc
N-Propanol	0.0000	264775	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	0.0000	30029	g/100cc
Ethanol	0.1161	61376	g/100cc
Acetone	0.0000	225305	g/100cc
Isopropyl Alcohol	0.0000	110709	g/100cc
N-Propanol	0.0000	248277	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

28

VOLATILES BAC CASEFILE WORKSHEET

Laboratory No.: 0.08

Item #

Analysis Date(s): 2/16/22

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Sample A-B Difference	Over-all Mean
Sample Results	0.0793	0.0793	0.0000	0.0793	0.0012	0.0799
(g/100cc)	0.0806	0.0805	0.0001	0.0805		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument information is stored centrally.

Refer to Instrument Method: Alcohol.m/.gcm, Volatiles.m/.gcm

Reporting of Results



Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.079	0.075	0.083	0.004

	Reported Result <hr style="border-top: 1px dashed black;"/> 0.079	
--	---	--

Calibration and control data are stored centrally.

Sample Name : 0.08 QA-A
 Laboratory : Meridian
 Injection Date : 2/16/2022 1:11:57 PM
 Vial # : 5
 Method Filename : C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
 Instrument #GC/HS : C12255750548 / C12595800409

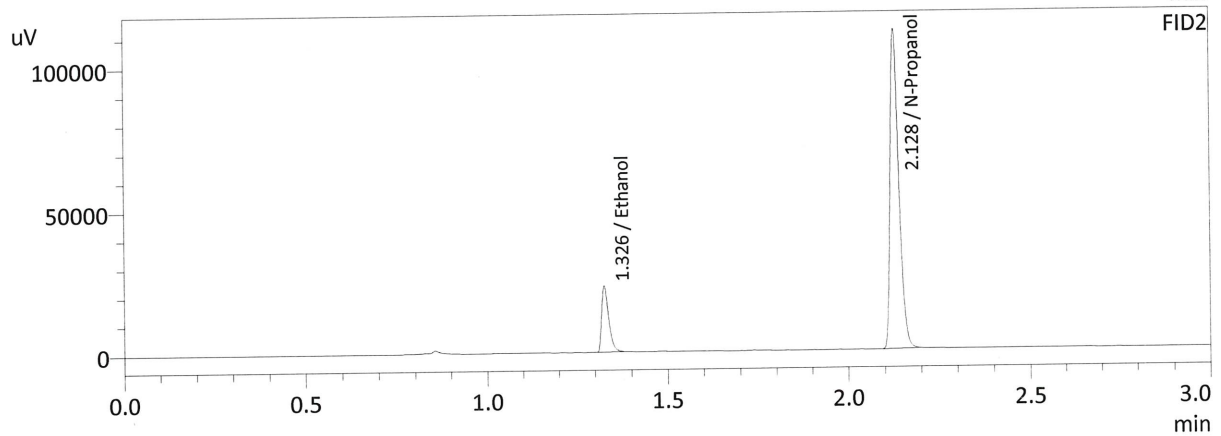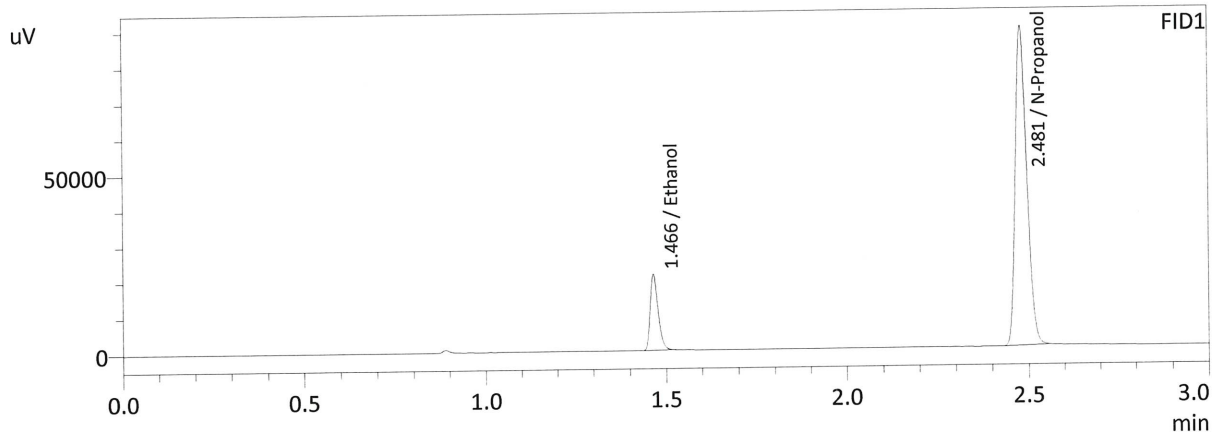

FID1



Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.0793	32342	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	196157	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.0793	30884	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	185157	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

NB

Sample Name : 0.08 QA-B
 Laboratory : Meridian
 Injection Date : 2/16/2022 1:20:40 PM
 Vial # : 6
 Method Filename : C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
 Instrument #GC/HS : C12255750548 / C12595800409

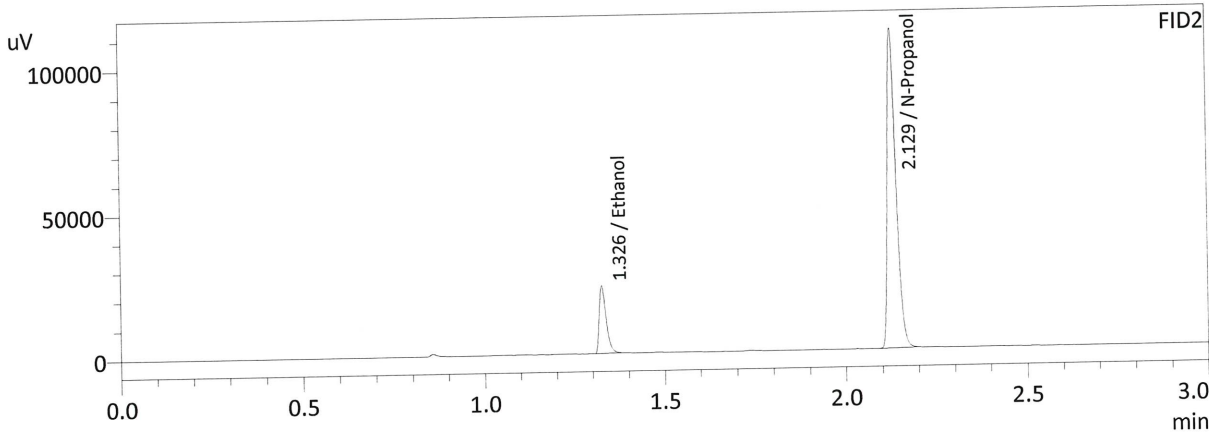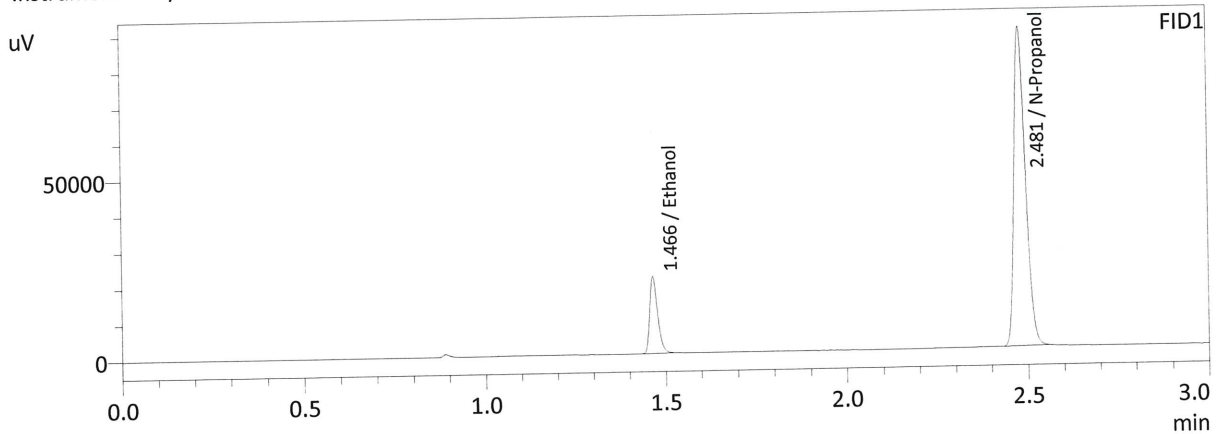

FID1

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.0806	32660	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	194746	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.0805	31140	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	183753	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

MB

VOLATILES BAC CASEFILE WORKSHEET

Laboratory No.: QC1-1

Item #

Analysis Date(s): 2/16/22

	Column 1 FID A	Column 2 B	FID	Column Precision	Mean Value	Sample A-B Difference	Over-all Mean
Sample Results	0.0733	0.0732		0.0001	0.0732	0.0011	0.0737
(g/100cc)	0.0743	0.0743		0.0000	0.0743		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument information is stored centrally.

Refer to Instrument Method: Alcohol.m/.gcm, Volatiles.m/.gcm

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%



Overall Mean (g/100cc)	Low	High	5% of Mean
0.073	0.069	0.077	0.004

	Reported Result
	0.073

Calibration and control data are stored centrally.

NB

Sample Name : QC-1-1-A
 Laboratory : Meridian
 Injection Date : 2/16/2022 12:55:47 PM
 Vial # : 3
 Method Filename : C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
 Instrument #GC/HS : C12255750548 / C12595800409

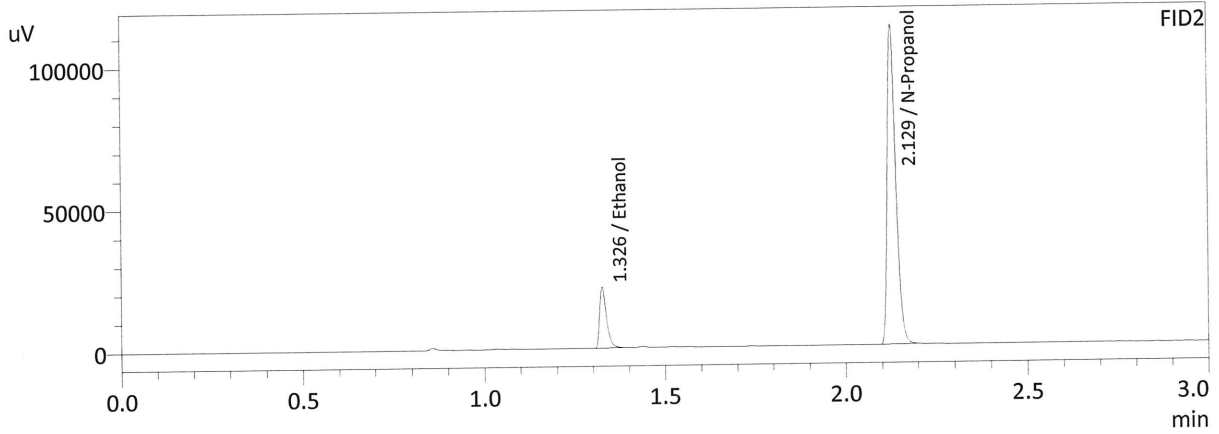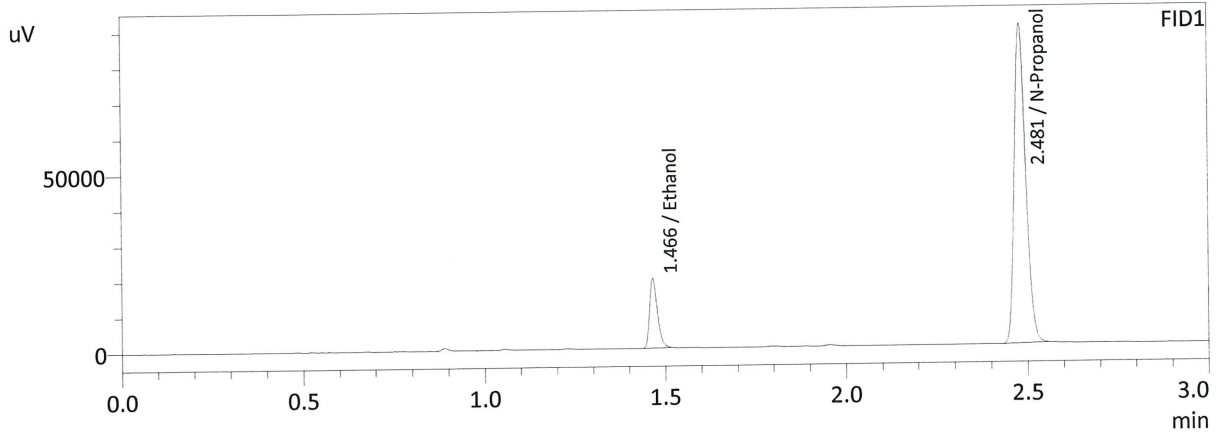

FID1



Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.0733	29910	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	197470	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.0732	28571	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	186218	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

MB

Sample Name : QC-1-1-B
 Laboratory : Meridian
 Injection Date : 2/16/2022 1:04:15 PM
 Vial # : 4
 Method Filename : C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
 Instrument #GC/HS : C12255750548 / C12595800409

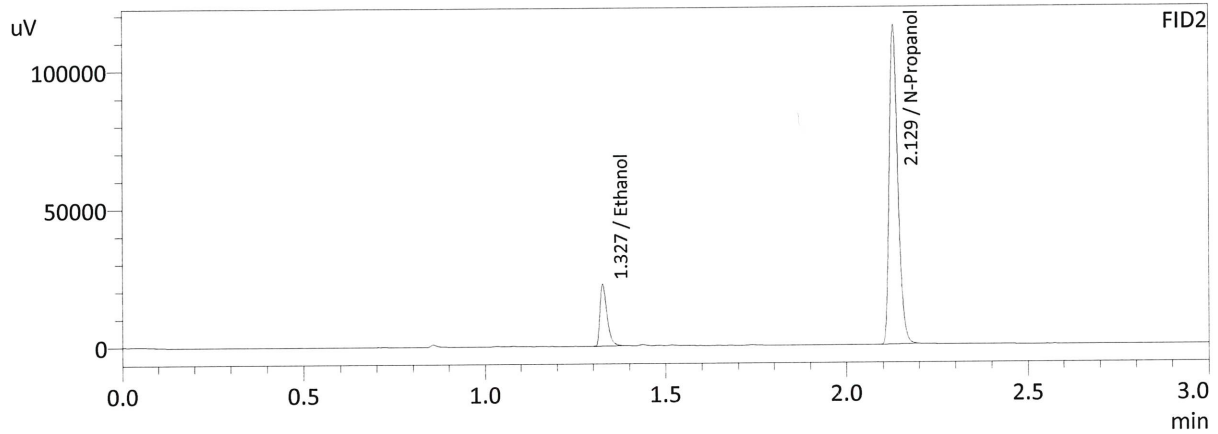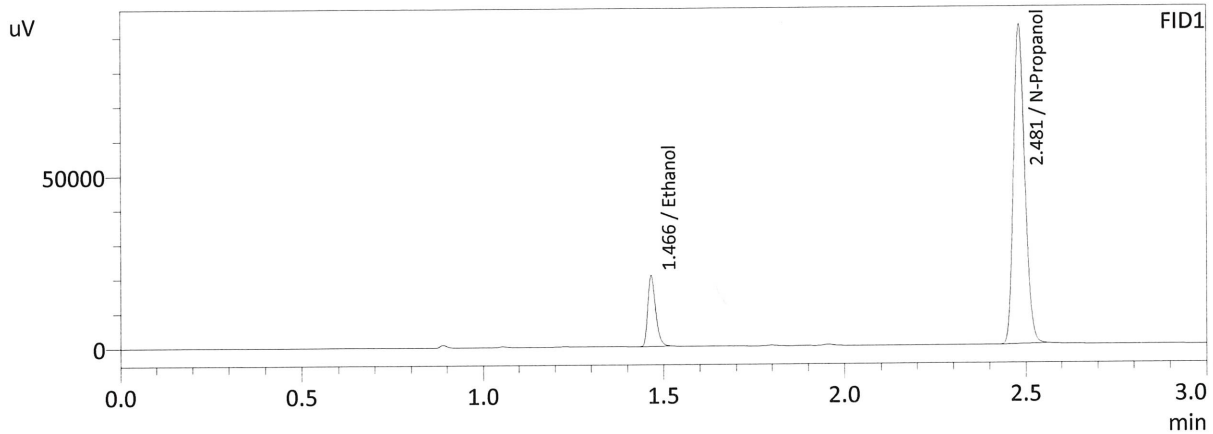

FID1

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.0743	31338	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	203689	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.0743	29942	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	192175	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

NB

VOLATILES BAC CASEFILE WORKSHEET

Laboratory No.: QC1-2

Item #

Analysis Date(s): 2/16/22

	Column 1 FID A	Column 2 B	FID Column Precision	Mean Value	Sample A-B Difference	Over-all Mean
Sample Results	0.0775	0.0785	0.0010	0.0780	0.0001	0.0779
(g/100cc)	0.0779	0.0780	0.0001	0.0779		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument information is stored centrally.

Refer to Instrument Method: Alcohol.m/.gcm, Volatiles.m/.gcm

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%



Overall Mean (g/100cc)	Low	High	5% of Mean
0.077	0.073	0.081	0.004

Reported Result	
0.077	

Calibration and control data are stored centrally.

NB

Sample Name : QC1-2-A
 Laboratory : Meridian
 Injection Date : 2/16/2022 6:49:53 PM
 Vial # : 47
 Method Filename : C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
 Instrument #GC/HS : C12255750548 / C12595800409

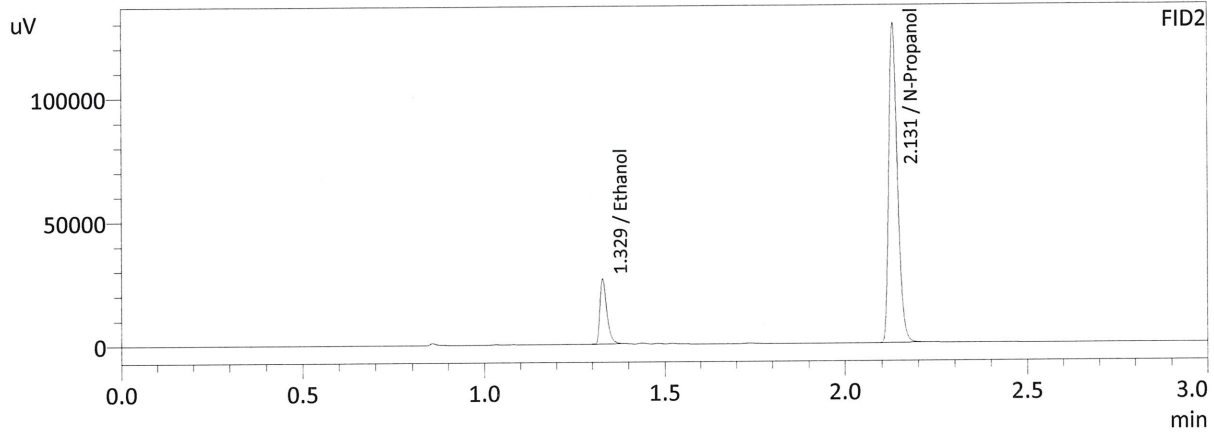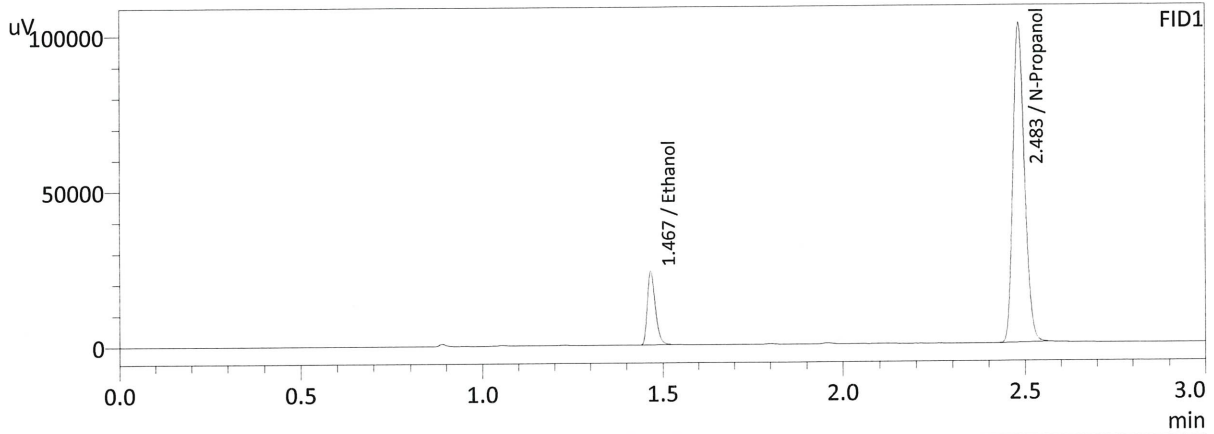

FID1



Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.0775	36444	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	226515	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.0785	35333	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	214004	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

NB

Sample Name : QC1-2-B
 Laboratory : Meridian
 Injection Date : 2/16/2022 6:59:04 PM
 Vial # : 48
 Method Filename : C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
 Instrument #GC/HS : C12255750548 / C12595800409

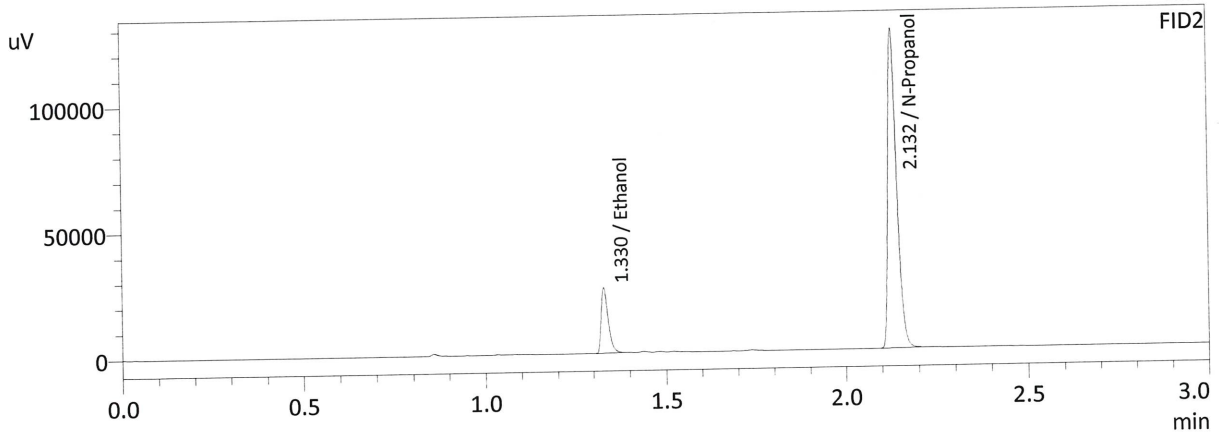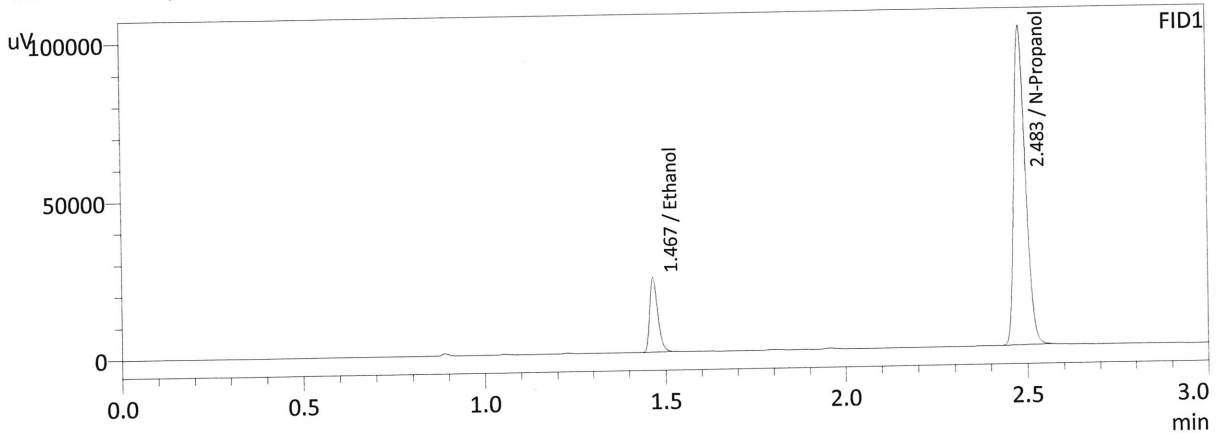

FID1

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.0779	36008	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	222572	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.0780	34509	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	210382	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

NB

VOLATILES BAC CASEFILE WORKSHEET

Laboratory No.: QC2-1

Item #

Analysis Date(s): 2/16/22

	Column 1 FID A	Column 2 FID B	FID	Column Precision	Mean Value	Sample A-B Difference	Over-all Mean
Sample Results	0.2137	0.2156		0.0019	0.2146	0.0016	0.2154
(g/100cc)	0.2158	0.2167		0.0009	0.2162		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument information is stored centrally.

Refer to Instrument Method: Alcohol.m/.gcm, Volatiles.m/.gcm

Reporting of Results

Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.215	0.204	0.226	0.011

	Reported Result	
	0.215	

Calibration and control data are stored centrally.





Revision: 1

Issue Date: 12/29/2021

Issuing Authority: Quality Manager

Sample Name : QC-2-1-A
 Laboratory : Meridian
 Injection Date : 2/16/2022 3:52:13 PM
 Vial # : 25
 Method Filename : C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
 Instrument #GC/HS : C12255750548 / C12595800409

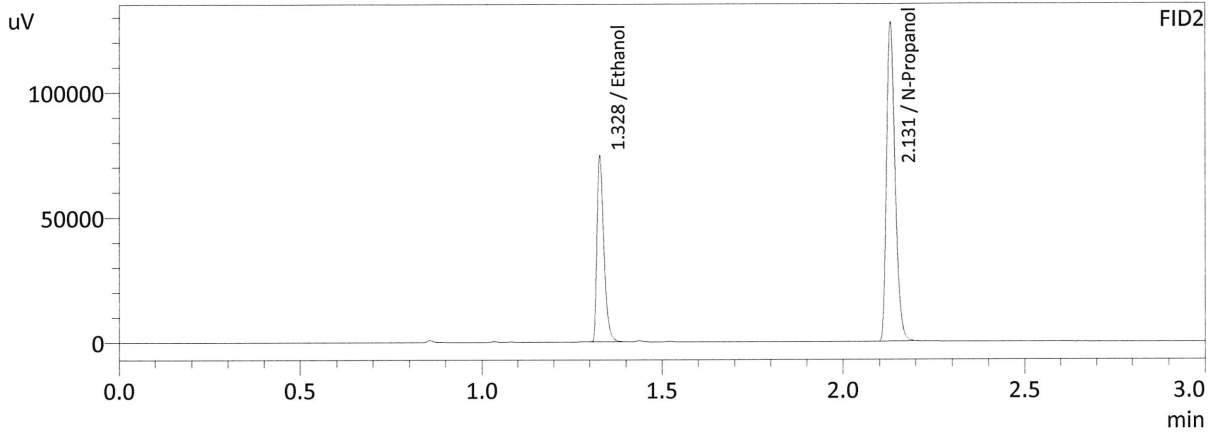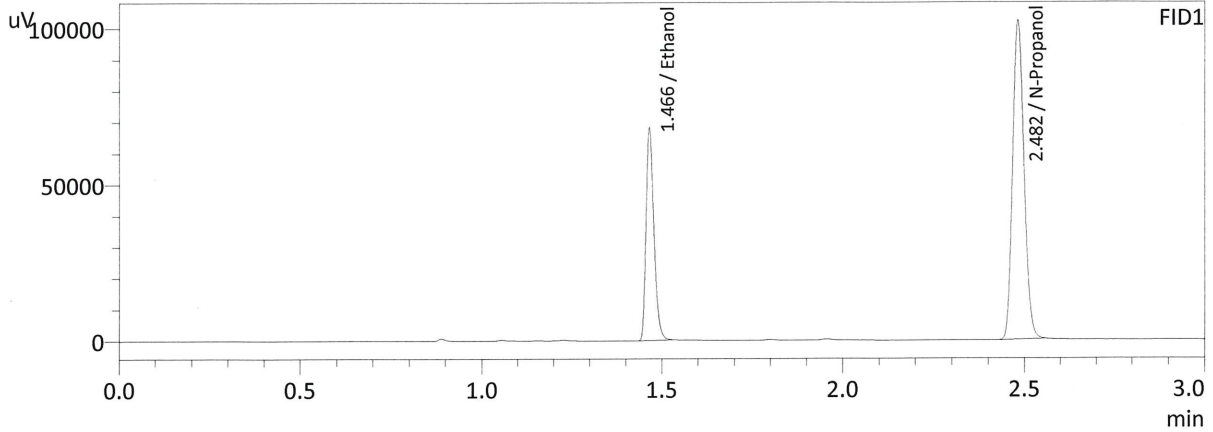

FID1



Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.2137	103662	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	224733	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.2156	98467	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	212013	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

NB

Sample Name : QC-2-1-B
 Laboratory : Meridian
 Injection Date : 2/16/2022 4:00:02 PM
 Vial # : 26
 Method Filename : C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
 Instrument #GC/HS : C12255750548 / C12595800409

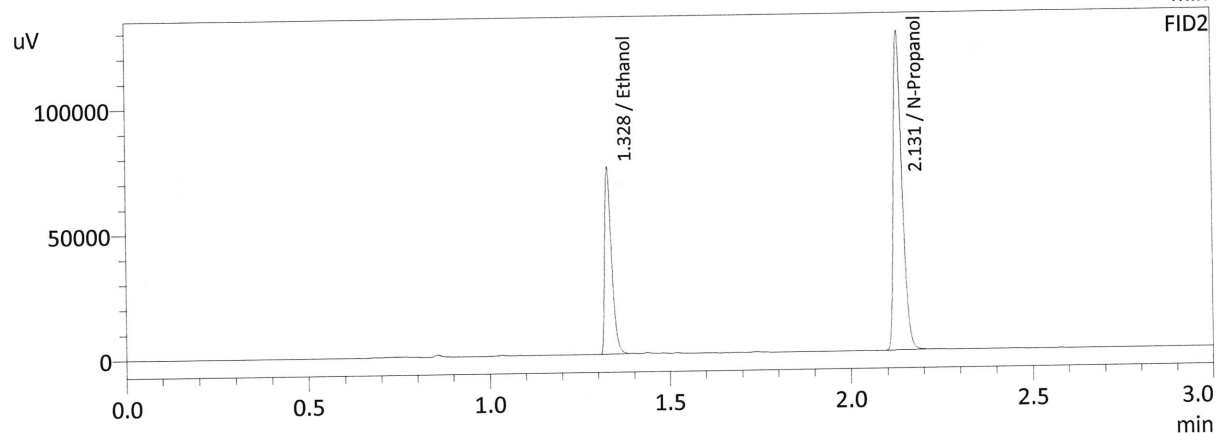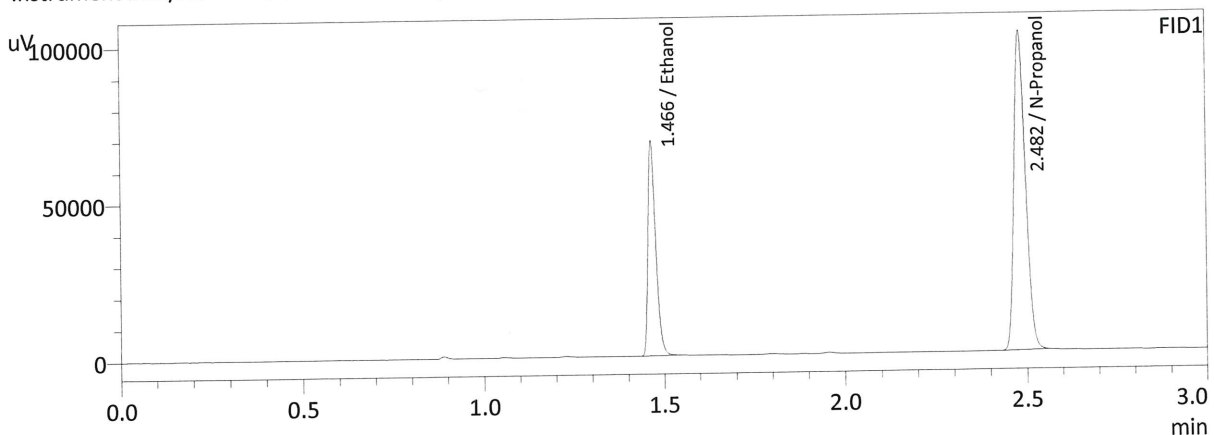

FID1

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.2158	104276	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	223834	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.2167	98636	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	211364	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

NB

VOLATILES BAC CASEFILE WORKSHEET

Laboratory No.: QC2-2

Item #

Analysis Date(s): 2/16/22

	Column 1 FID A	Column 2 FID B	FID	Column Precision	Mean Value	Sample A-B Difference	Over-all Mean
Sample Results	0.2173	0.2184		0.0011	0.2178	0.0009	0.2173
(g/100cc)	0.2163	0.2175		0.0012	0.2169		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument information is stored centrally.

Refer to Instrument Method: Alcohol.m/.gcm, Volatiles.m/.gcm

Reporting of Results


Uncertainty of Measurement (UM%): 5.00%

Overall Mean (g/100cc)	Low	High	5% of Mean
0.217	0.206	0.228	0.011

Reported Result	
0.217	

Calibration and control data are stored centrally.

Sample Name : QC2-2-A
 Laboratory : Meridian
 Injection Date : 2/16/2022 8:59:07 PM
 Vial # : 63
 Method Filename : C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
 Instrument #GC/HS : C12255750548 / C12595800409

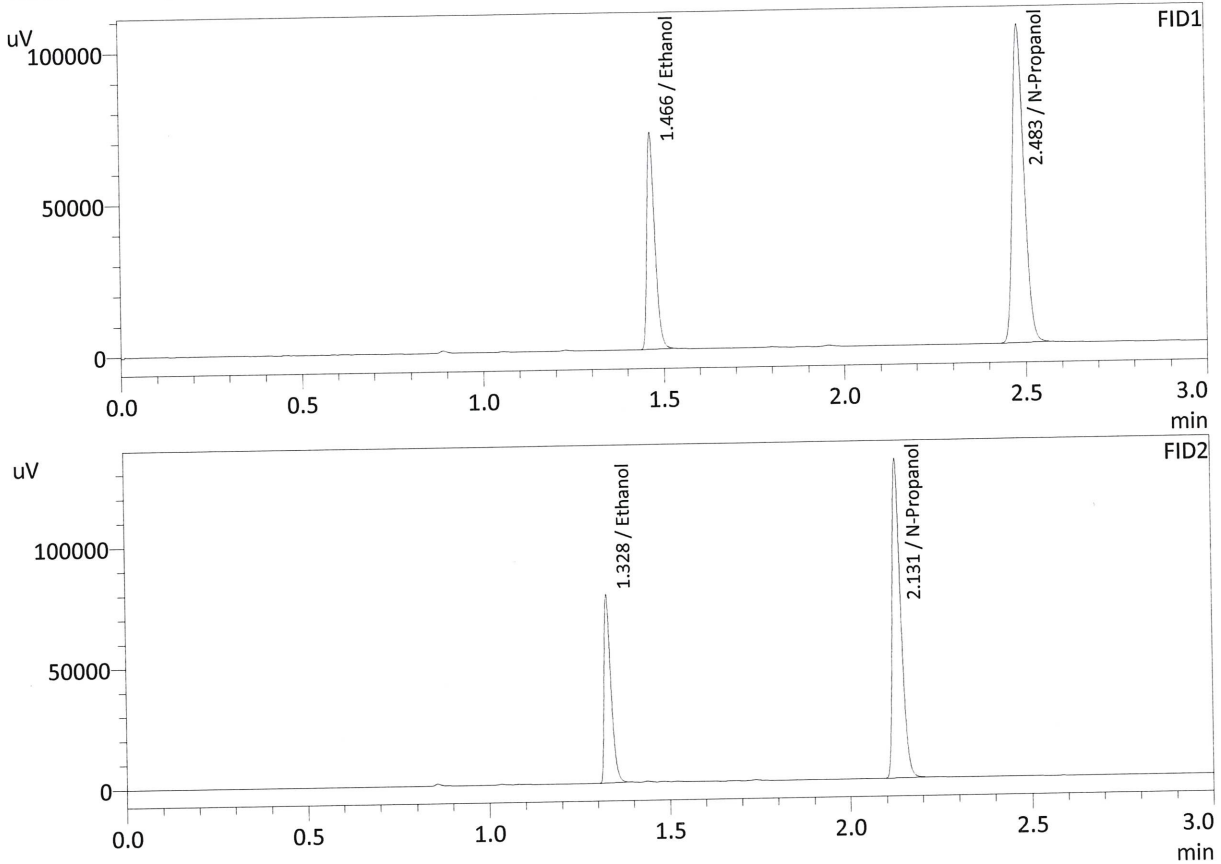

FID1



Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.2173	108687	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	231638	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.2184	102707	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	218325	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

NB

Sample Name : QC2-2-B
 Laboratory : Meridian
 Injection Date : 2/16/2022 9:06:41 PM
 Vial # : 64
 Method Filename : C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
 Instrument #GC/HS : C12255750548 / C12595800409

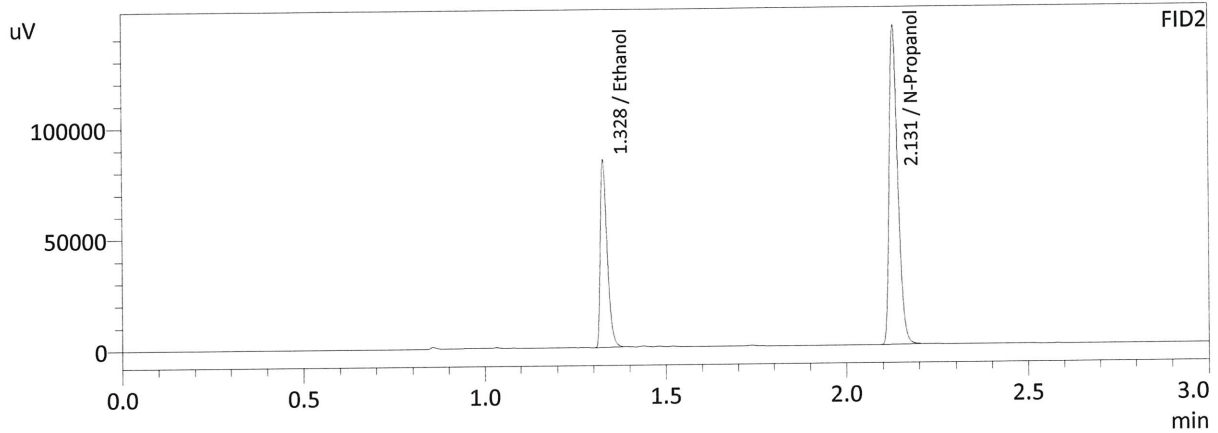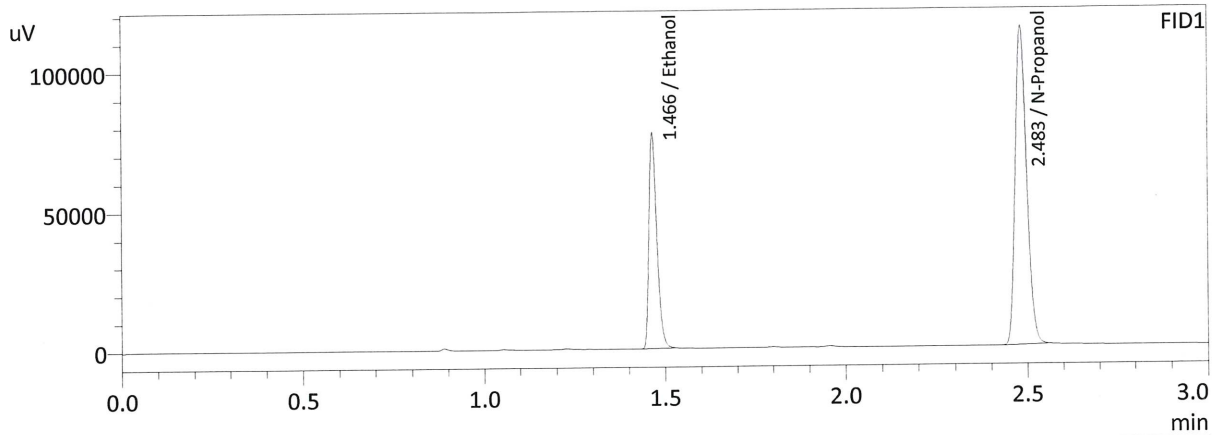

FID1



Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.2163	117813	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	252262	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.2175	111477	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	237888	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

NB

Sample Name : INT STD BLK
 Laboratory : Meridian
 Injection Date : 2/16/2022 9:14:27 PM
 Vial # : 65
 Method Filename : C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
 Instrument #GC/HS : C12255750548 / C12595800409

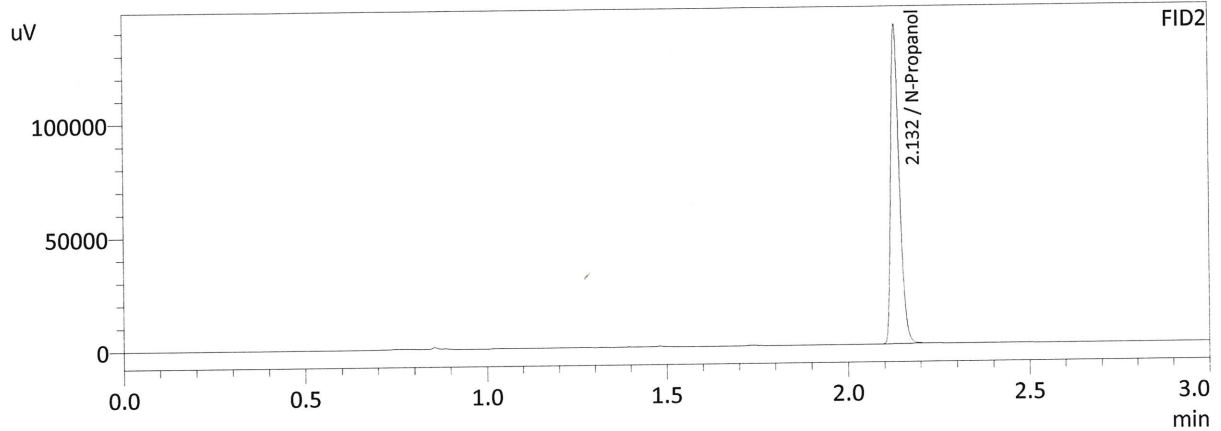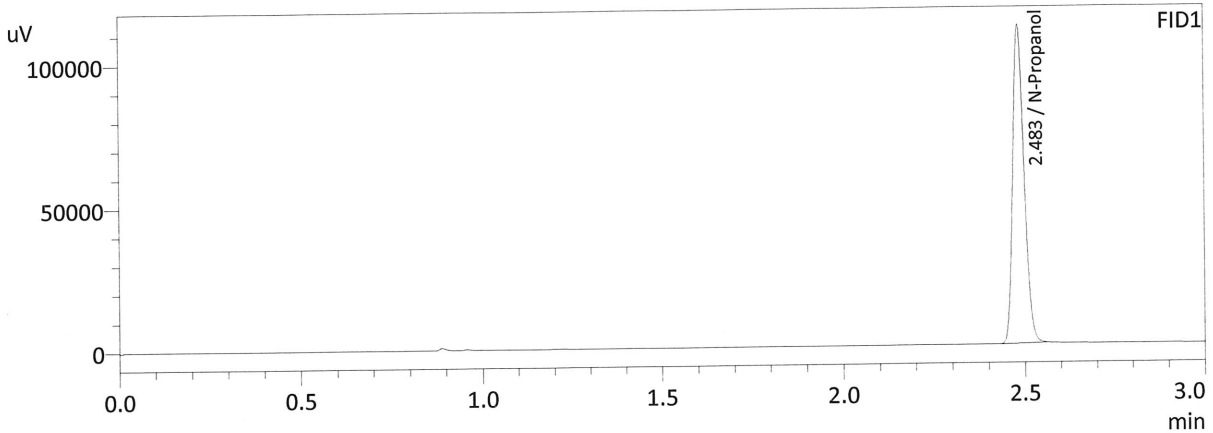

FID1

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	245129	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	--	--	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	232119	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc



NB

Meridian Blood Alcohol Analysis Batch Table

Shimadzu GC-2030 Serial #C12255750548
 Shimadzu HS-20 Serial #C12595800409
 Lab Solutions Software Ver. 5.99
 Copyright (C) 2008-2020 Shimadzu Corporation

Vial#	Sample Name	Method File
1	INT STD BLK 1	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
2	ED VOLATILES FN 0710	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
3	QC-1-1-A	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
4	QC-1-1-B	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
5	0.08 QA-A	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
6	0.08 QA-B	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
7	M2022-0460-1-A	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
8	M2022-0460-1-B	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
9	M2022-0470-1-A	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
10	M2022-0470-1-B	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
11	M2022-0476-2-A	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
12	M2022-0476-2-B	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
13	M2022-0479-1-A	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
14	M2022-0479-1-B	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
15	M2022-0502-1-A	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
16	M2022-0502-1-B	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
17	M2022-0504-1-A	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
18	M2022-0504-1-B	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
19	M2022-0505-1-A	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
20	M2022-0505-1-B	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
21	M2022-0522-1-A	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
22	M2022-0522-1-B	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
23	M2022-0544-1-A	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
24	M2022-0544-1-B	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
25	QC-2-1-A	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
26	QC-2-1-B	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
27	M2022-0548-1-A	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
28	M2022-0548-1-B	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
29	M2022-0549-1-A	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
30	M2022-0549-1-B	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
31	M2022-0550-1-A	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
32	M2022-0550-1-B	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
33	M2022-0566-1-A	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
34	M2022-0566-1-B	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
35	M2022-0598-1-A	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
36	M2022-0598-1-B	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
37	M2022-0599-1-A	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
38	M2022-0599-1-B	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
39	M2022-0614-1-A	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
40	M2022-0614-1-B	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
41	M2022-0614-2-A	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
42	M2022-0614-2-B	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
43	M2022-0614-3-A	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
44	M2022-0614-3-B	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
45	M2022-0614-4-A	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
46	M2022-0614-4-B	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
47	QC1-2-A	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
48	QC1-2-B	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
49	M2022-0636-1-A	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
50	M2022-0636-1-B	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
51	M2022-0637-1-A	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
52	M2022-0637-1-B	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
53	M2022-0638-1-A	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
54	M2022-0638-1-B	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
55	M2022-0639-1-A	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
56	M2022-0639-1-B	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
57	M2022-0640-1-A	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
58	M2022-0640-1-B	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
59	M2022-0641-1-A	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
60	M2022-0641-1-B	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
61	P2022-0333-1-A	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
62	P2022-0333-1-B	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
63	QC2-2-A	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
64	QC2-2-B	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
65	INT STD BLK	C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM

Sample Name : DFE 111914OM
 Laboratory : Meridian
 Injection Date : 2/16/2022 9:40:45 PM
 Vial # : 66
 Method Filename : C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
 Instrument #GC/HS : C12255750548 / C12595800409

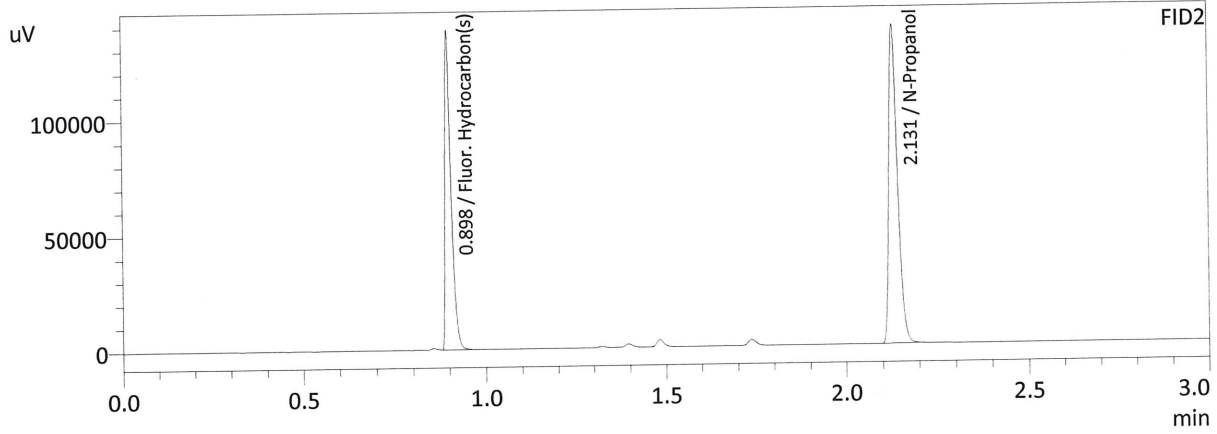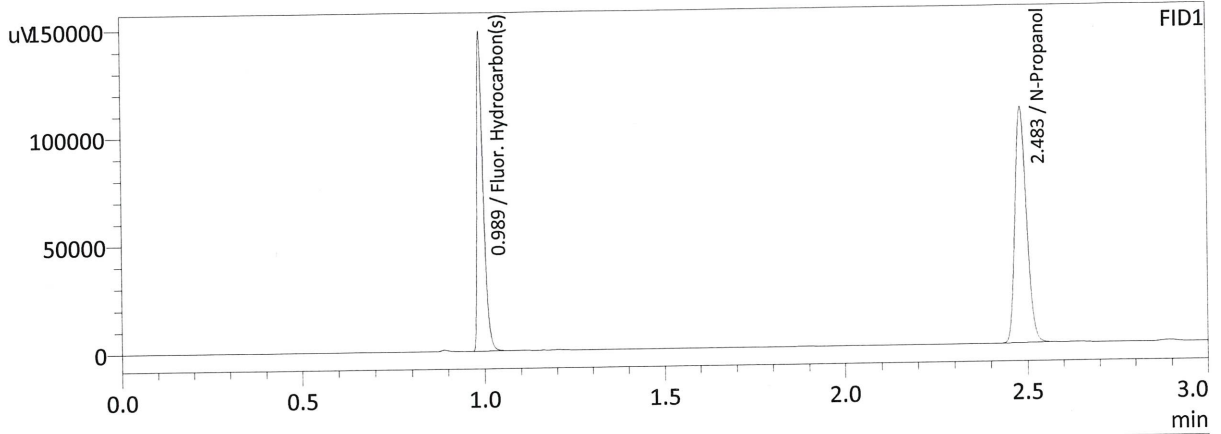

FID1



Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	241438	g/100cc
Fluor. Hydrocarbon(s)	0.0000	175998	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	--	--	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	228132	g/100cc
Fluor. Hydrocarbon(s)	0.0000	158989	g/100cc

MB

Sample Name : ISTD BLK
 Laboratory : Meridian
 Injection Date : 2/16/2022 9:47:52 PM
 Vial # : 67
 Method Filename : C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
 Instrument #GC/HS : C12255750548 / C12595800409

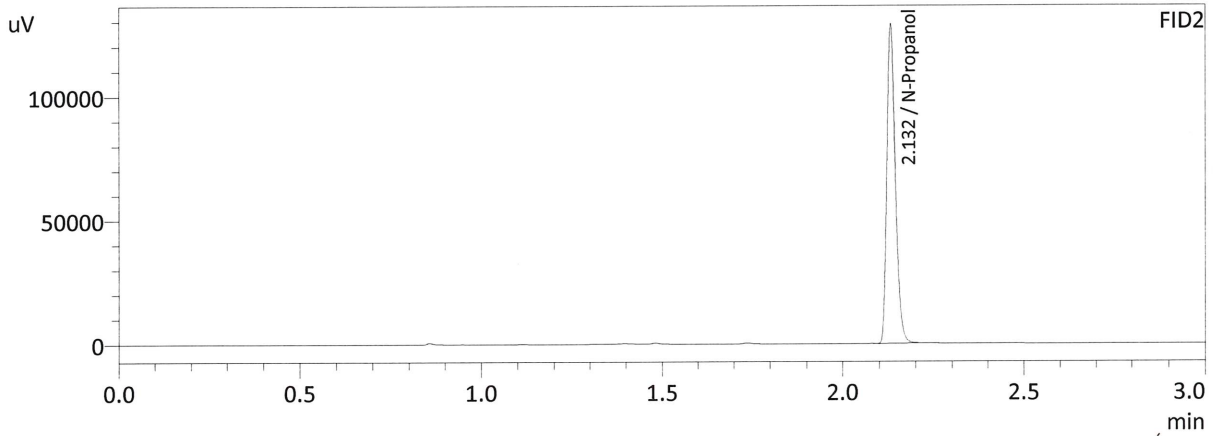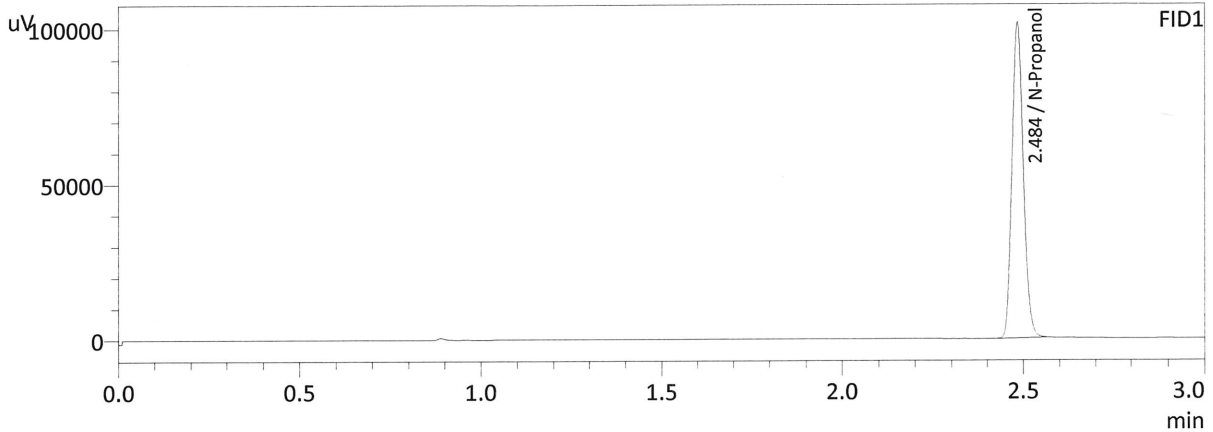

FID1

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	224098	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	--	--	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	212192	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc



Meridian Blood Alcohol Analysis Batch Table

Shimadzu GC-2030 Serial #C12255750548
Shimadzu HS-20 Serial #C12595800409
Lab Solutions Software Ver. 5.99
Copyright (C) 2008-2020 Shimadzu Corporation

Vial#	Sample Name	Sample Type	Level#	Method File
66	DFE 111914OM	0:Unknown	0	s\Data\220216\CALIBRATION\AI
67	ISTD BLK	0:Unknown	0	s\Data\220216\CALIBRATION\AI



Sample Name : TFE 111914
 Laboratory : Meridian
 Injection Date : 2/17/2022 9:12:07 AM
 Vial # : 1
 Method Filename : C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
 Instrument #GC/HS : C12255750548 / C12595800409

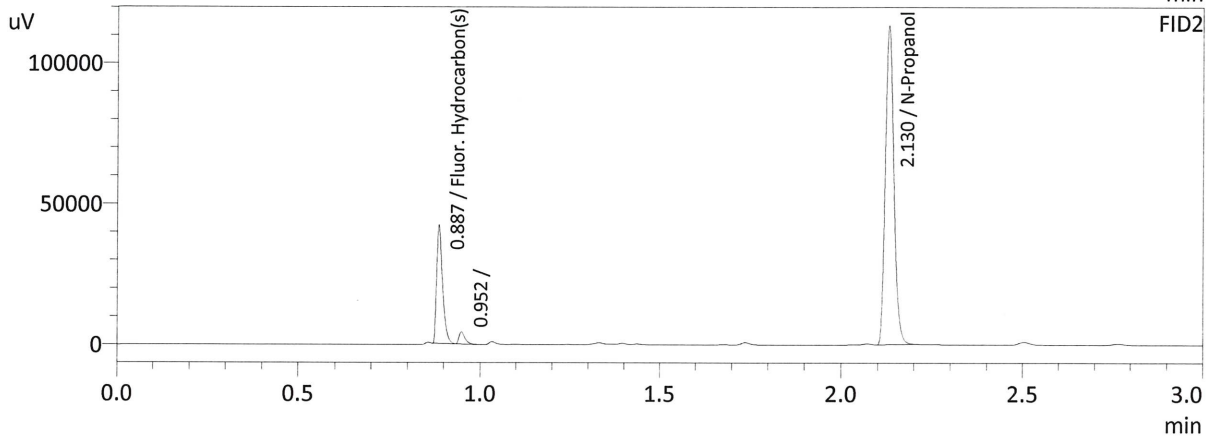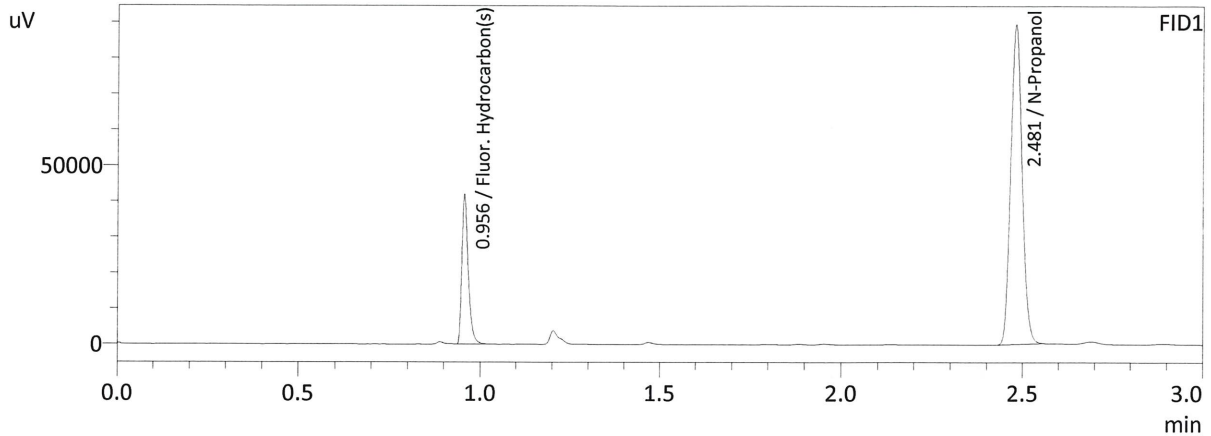

FID1



Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	198729	g/100cc
Fluor. Hydrocarbon(s)	0.0000	50788	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	--	--	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	187783	g/100cc
Fluor. Hydrocarbon(s)	0.0000	48056	g/100cc

NB

Sample Name : ISTD BLK
 Laboratory : Meridian
 Injection Date : 2/17/2022 9:19:18 AM
 Vial # : 2
 Method Filename : C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
 Instrument #GC/HS : C12255750548 / C12595800409

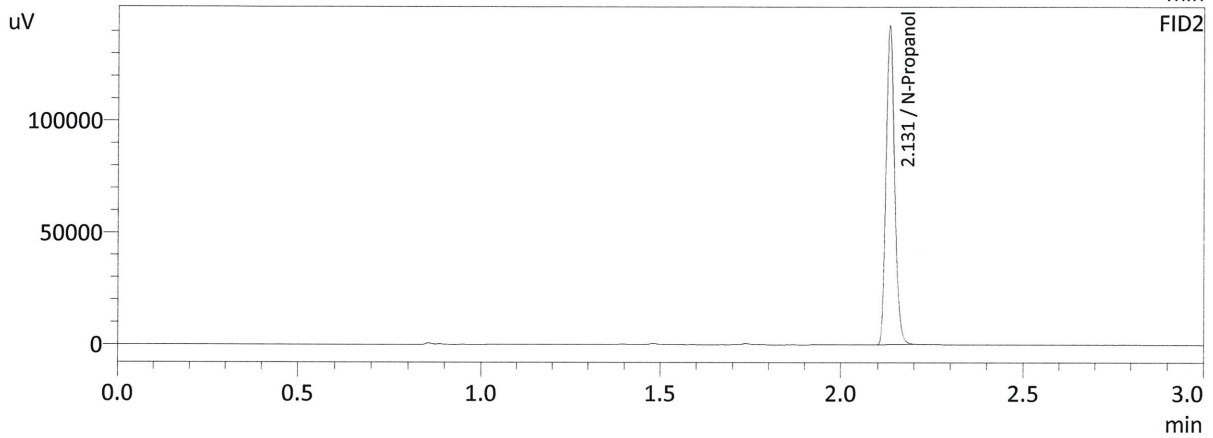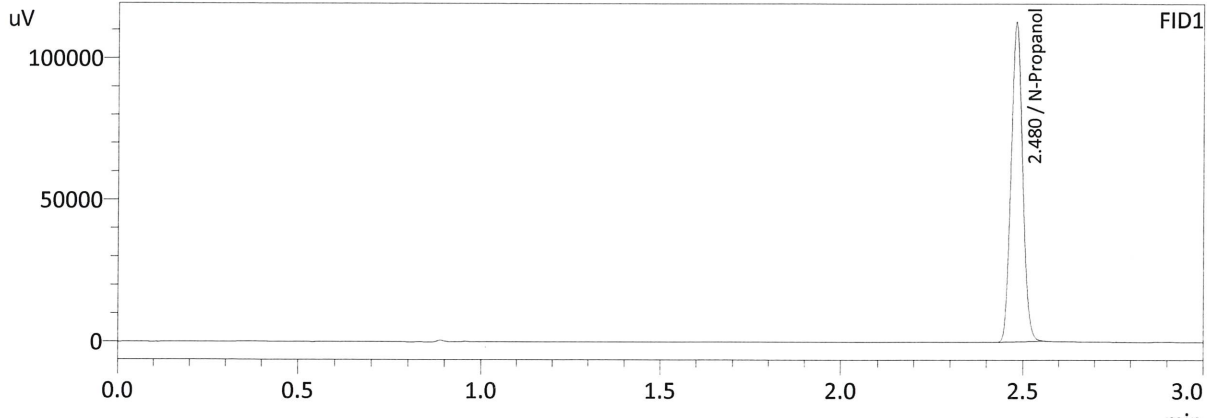

FID1

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	249555	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	--	--	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	235778	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc



MB

Meridian Blood Alcohol Analysis Batch Table

Shimadzu GC-2030 Serial #C12255750548
Shimadzu HS-20 Serial #C12595800409
Lab Solutions Software Ver. 5.99
Copyright (C) 2008-2020 Shimadzu Corporation

Vial#	Sample Name	Sample Type	Level#	Method File
1	TFE 111914	0:Unknown	0	s\Data\220216\CALIBRATION\AI
2	ISTD BLK	0:Unknown	0	s\Data\220216\CALIBRATION\AI

Sample Name : ISTD BLK A
 Laboratory : Meridian
 Injection Date : 2/17/2022 10:34:54 AM
 Vial # : 3
 Method Filename : C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
 Instrument #GC/HS : C12255750548 / C12595800409

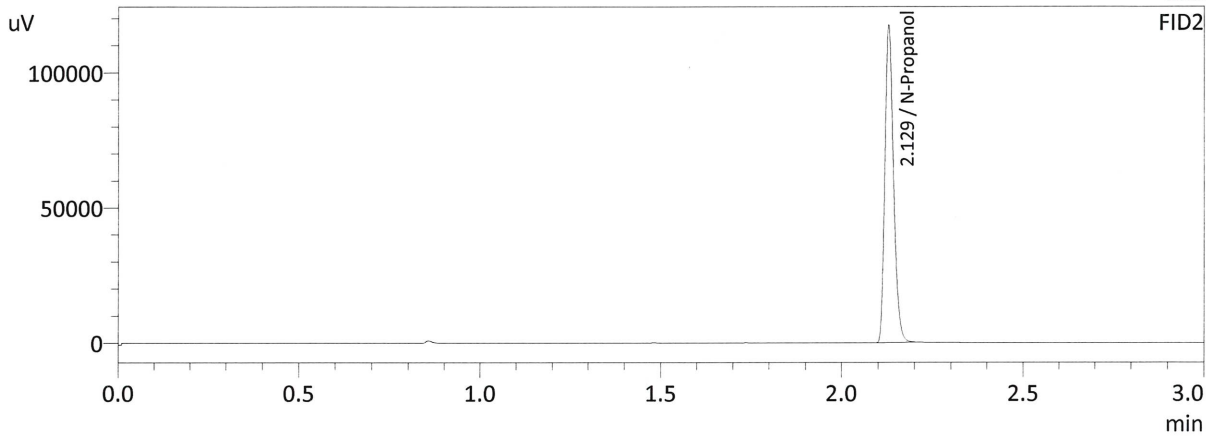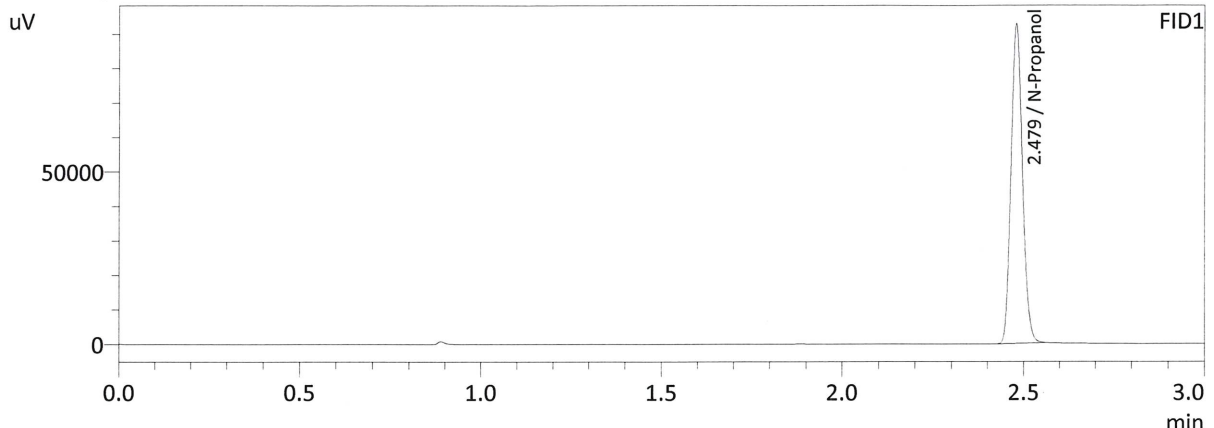

FID1



Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	205688	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	--	--	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	194617	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

NB

Sample Name : ISTD BLK B
 Laboratory : Meridian
 Injection Date : 2/17/2022 10:58:25 AM
 Vial # : 6
 Method Filename : C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
 Instrument #GC/HS : C12255750548 / C12595800409

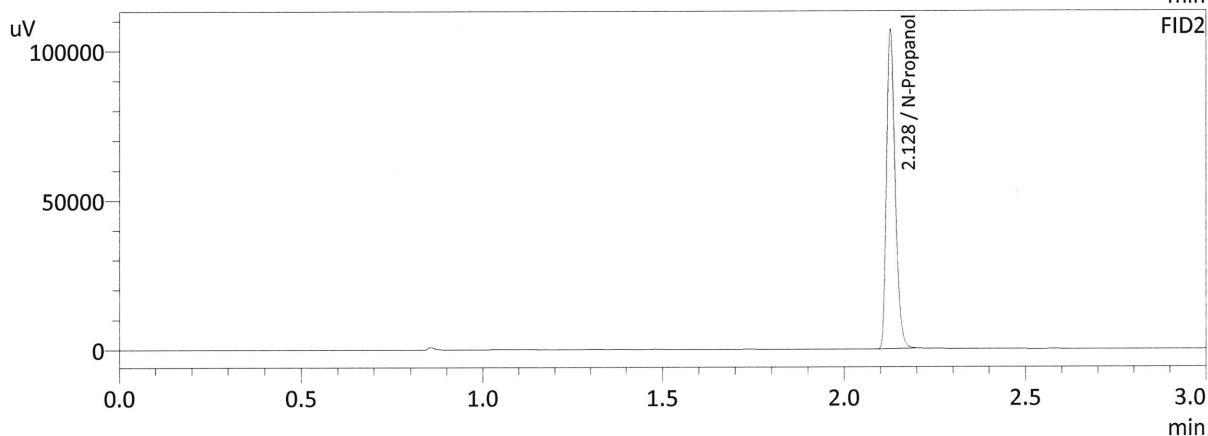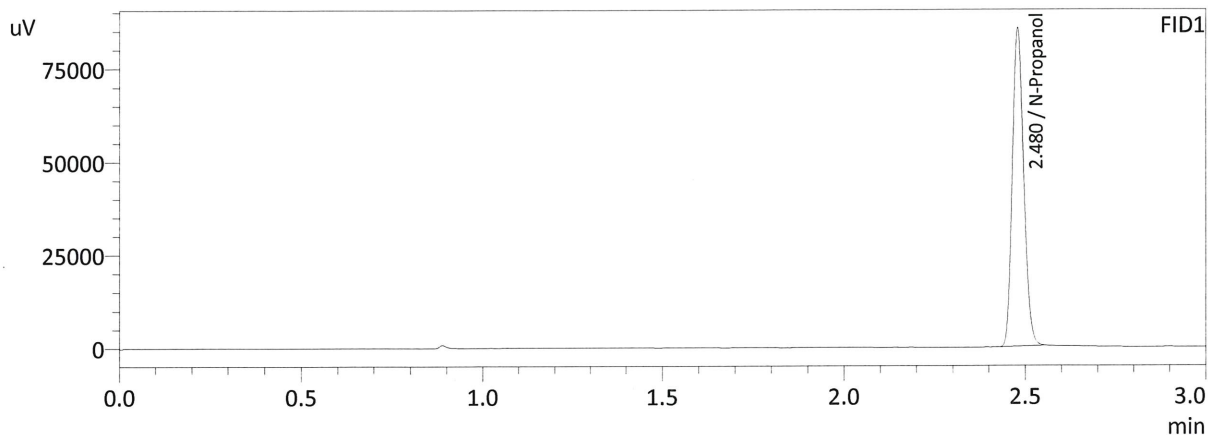

FID1



Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	187459	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	--	--	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	177774	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

MB

Sample Name : ISTD BLK C
 Laboratory : Meridian
 Injection Date : 2/17/2022 11:21:47 AM
 Vial # : 9
 Method Filename : C:\LabSolutions\Data\220216\CALIBRATION\ALCOHOL.GCM
 Instrument #GC/HS : C12255750548 / C12595800409

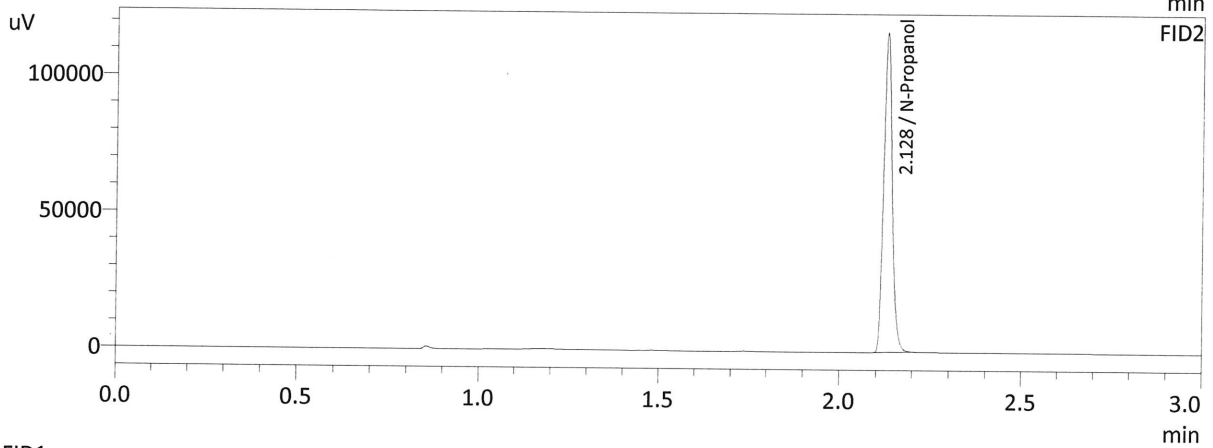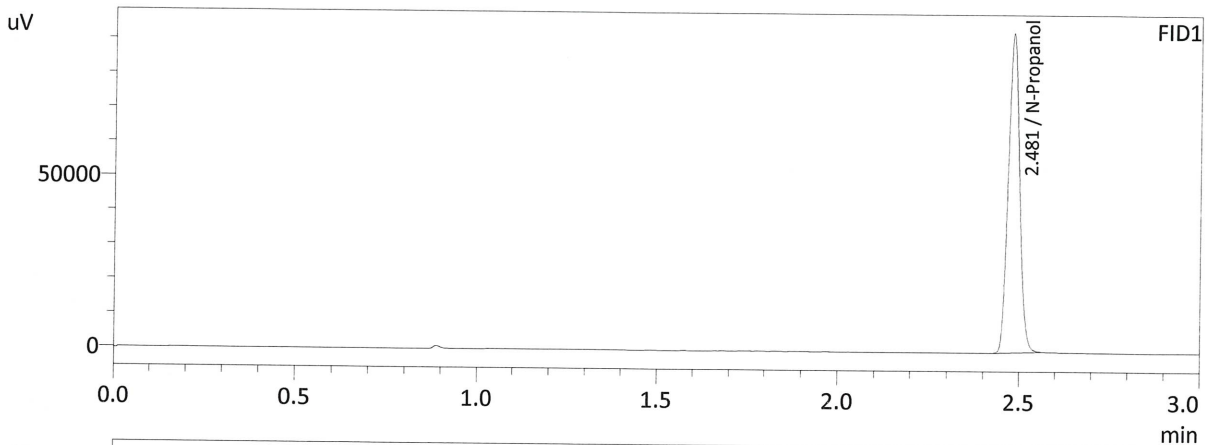

FID1

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	204773	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	--	--	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	193867	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

NB

Meridian Blood Alcohol Analysis Batch Table

Shimadzu GC-2030 Serial #C12255750548
Shimadzu HS-20 Serial #C12595800409
Lab Solutions Software Ver. 5.99
Copyright (C) 2008-2020 Shimadzu Corporation

Vial#	Sample Name	Sample Type	Level#	Method File
3	ISTD BLK A	0:Unknown	0	s\Data\220216\CALIBRATION\AI
4	M2022-0479-1A QUAL	0:Unknown	0	s\Data\220216\CALIBRATION\AI
5	M2022-0479-1B QUAL	0:Unknown	0	s\Data\220216\CALIBRATION\AI
6	ISTD BLK B	0:Unknown	0	s\Data\220216\CALIBRATION\AI
7	M2022-0502-1A QUAL	0:Unknown	0	s\Data\220216\CALIBRATION\AI
8	M2022-0502-1B QUAL	0:Unknown	0	s\Data\220216\CALIBRATION\AI
9	ISTD BLK C	0:Unknown	0	s\Data\220216\CALIBRATION\AI

