




**Worklist: 6330**

<u>LAB CASE</u>	<u>ITEM</u>	<u>ITEM TYPE</u>	<u>DESCRIPTION</u>
C2023-0753	1	BCK	Alcohol Analysis
C2023-0759	1	BCK	Alcohol Analysis
C2023-0760	1	BCK	Alcohol Analysis
C2023-0760	2	BCK	Alcohol Analysis
C2023-0761	1	BCK	Alcohol Analysis
C2023-0761	2	BCK	Alcohol Analysis
C2023-0761	3	BCK	Alcohol Analysis
C2023-0761	4	BCK	Alcohol Analysis

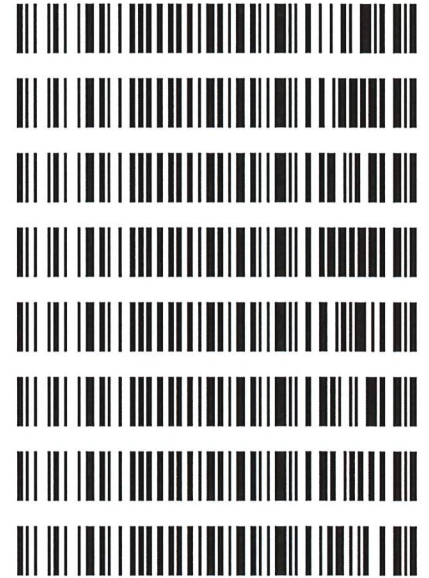

# Region 1 CDA Blood Alcohol Analysis Batch Table

Shimadzu GC-2030 Serial #C12255850700  
 Shimadzu HS-20 Serial #C12595700181  
 Lab Solutions DB Software Ver. 6.111  
 Copyright (C) 2008-2020 Shimadzu Corporation

Vial#	Sample Name	Sample Type	Level#	Method File
78	INT STD BLK 5	0:Unknown	0	ALCOHOL.gcm
79	INT STD BLK 6	0:Unknown	0	ALCOHOL.gcm
80	INT STD BLK 7	0:Unknown	0	ALCOHOL.gcm
81	INT STD BLK 8	0:Unknown	0	ALCOHOL.gcm
82	INT STD BLK 9	0:Unknown	0	ALCOHOL.gcm
83	INT STD BLK 10	0:Unknown	0	ALCOHOL.gcm
1	INT STD BLK 1	0:Unknown	0	ALCOHOL.gcm
2	MULTI-COMP MIX	1:Standard:(R)	6	ALCOHOL.gcm
3	INT STD BLK 2	0:Unknown	0	ALCOHOL.gcm
4	QC-1-1	0:Unknown	0	ALCOHOL.gcm
5	QC-1-1-B	0:Unknown	0	ALCOHOL.gcm
6	QC-2-1	0:Unknown	0	ALCOHOL.gcm
7	QC-2-1-B	0:Unknown	0	ALCOHOL.gcm
8	0.08 QA	0:Unknown	0	ALCOHOL.gcm
9	0.08 QA - B	0:Unknown	0	ALCOHOL.gcm
10	C2023-0753-1	0:Unknown	0	ALCOHOL.gcm
11	C2023-0753-1-B	0:Unknown	0	ALCOHOL.gcm
12	C2023-0759-1	0:Unknown	0	ALCOHOL.gcm
13	C2023-0759-1-B	0:Unknown	0	ALCOHOL.gcm
14	C2023-0760-1	0:Unknown	0	ALCOHOL.gcm
15	C2023-0760-1-B	0:Unknown	0	ALCOHOL.gcm
16	C2023-0760-2	0:Unknown	0	ALCOHOL.gcm
17	C2023-0760-2-B	0:Unknown	0	ALCOHOL.gcm
18	C2023-0761-1	0:Unknown	0	ALCOHOL.gcm
19	C2023-0761-1-B	0:Unknown	0	ALCOHOL.gcm
20	C2023-0761-2	0:Unknown	0	ALCOHOL.gcm
21	C2023-0761-2-B	0:Unknown	0	ALCOHOL.gcm
22	C2023-0761-3	0:Unknown	0	ALCOHOL.gcm
23	C2023-0761-3-B	0:Unknown	0	ALCOHOL.gcm
24	C2023-0761-4	0:Unknown	0	ALCOHOL.gcm
25	C2023-0761-4-B	0:Unknown	0	ALCOHOL.gcm
26	QC-1-2	0:Unknown	0	ALCOHOL.gcm
27	QC-1-2-B	0:Unknown	0	ALCOHOL.gcm
28	QC-2-2	0:Unknown	0	ALCOHOL.gcm
29	QC-2-2-B	0:Unknown	0	ALCOHOL.gcm
30	INT STD BLK 3	0:Unknown	0	ALCOHOL.gcm
31	INT STD BLK 4	0:Unknown	0	ALCOHOL.gcm

99

### Quantitative Analysis for Ethanol & Qualitative Analysis for Other Volatiles

*Analytical Method(s): 1.0*

*Device: Hamilton MICROLAB Liquid Processor/Dilutor Serial Number: ML600HC11379*

Volatiles Quality Assurance Controls

Run Date(s): 4/8/2023

Calibration Date: (if different) 4/5/2023

Worklist #: 6330

Control level	Expiration	Lot #	Target Value	Acceptable Range	Overall Results	
Level 1	Feb-25	2101199	0.0808	0.0727 - 0.0889	0.0799 g/100cc	
					0.0822 g/100cc	
					g/100cc	
Level 2	Jul-23	1907007	0.2170	0.1953 - 0.2387	0.1963 g/100cc	
					0.2032 g/100cc	
					g/100cc	
<b>Multi-Component mixture:</b>		<b>Exp:</b>	July 31, 2024	<b>Lot #</b>	FN04231907	OK
<b>Curve Fit:</b>			<b>Column 1</b>	0.99955	<b>Column2</b>	0.99943

#### Ethanol Calibration Reference Material

Calibrator level	Target Value	Acceptable Range	Column 1	Column 2	Precision	Mean
50	0.050	0.045 - 0.055	0.0539	0.0546	0.0007	0.0542
100	0.100	0.090 - 0.110	0.0999	0.0997	0.0002	0.0998
200	0.200	0.180 - 0.220	0.1953	0.1945	0.0008	0.1949
300	0.300	0.270 - 0.330			0	#DIV/0!
400	0.400	0.360 - 0.440	0.3965	0.3964	0.0001	0.3964
500	0.500	0.450 - 0.550	0.5042	0.5045	0.0003	0.5043

#### Aqueous Controls

Control level	Target Value	Acceptable Range	Overall Results
80	0.080	0.076 - 0.084	0.082 g/100cc

**REVIEWED**

*By Rachel Cutler at 10:23 am, Apr 11, 2023*

Revision: 5

Issue Date: 07/05/2022

Issuing Authority: Quality Manager

99

### Internal Standard Monitoring Worksheet

<b>Worklist #:</b>	<b>6330</b>	<b>Run Date(s):</b>	<b>4/8/2023</b>
--------------------	-------------	---------------------	-----------------

Internal Standard Solution: Lot# A014463901	Prep Date: 3/14/2023	Exp Date: 9/14/2023
---	----------------------	---------------------



Sample Name	Column 1 Value	Column 2 Value
0.080	252836	273488
0.080	256221	277304
QC1	254836	275225
QC1	256196	277127
QC1	297068	321152
QC1	300413	324789
QC1		
QC1		
QC2	257504	278396
QC2	259613	280443
QC2	299319	323661
QC2	292099	315712
QC2		
QC2		

	Average	(-)20%	(+)20%
Column 1	272610.5	218088.4	327132.6
Column 2	294729.7	235783.8	353675.6



99

Sample Name : INT STD BLK 1  
 Laboratory : Coeur d' Alene Lab  
 Injection Date : 4/8/2023 5:04:44 PM  
 Vial # : 1  
 Method Filename : Default Project - ALCOHOL.gcm  
 Instrument #GC/HS : C12255850700 / C12595700181

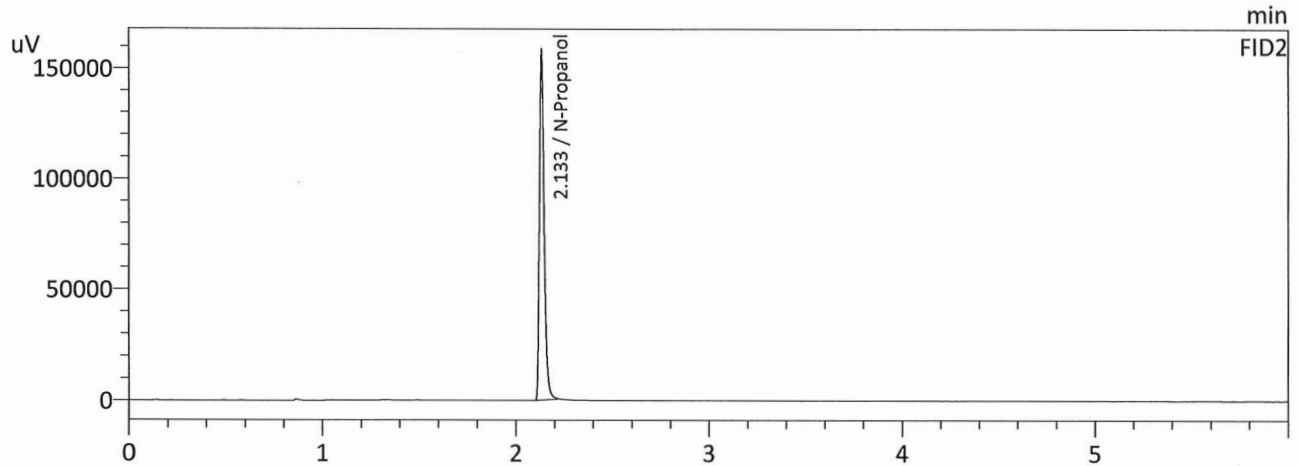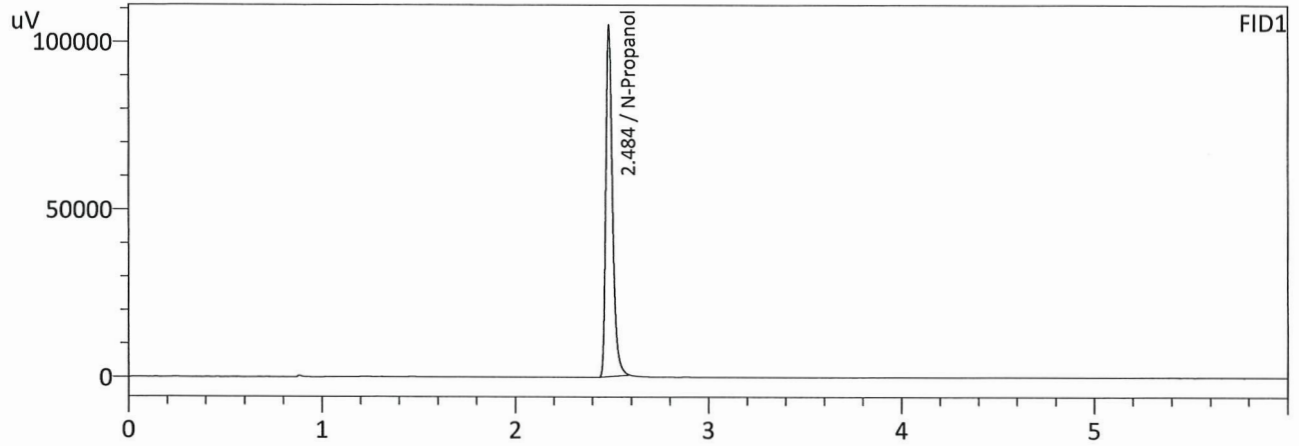

FID1



Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	250074	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	--	--	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	269678	g/100cc
Flour. Hydrocarbon(s)	--	--	g/100cc

99

Sample Name : MULTI-COMP MIX  
 Laboratory : Coeur d' Alene Lab  
 Injection Date : 4/8/2023 5:13:26 PM  
 Vial # : 2  
 Method Filename : Default Project - ALCOHOL.gcm  
 Instrument #GC/HS : C12255850700 / C12595700181

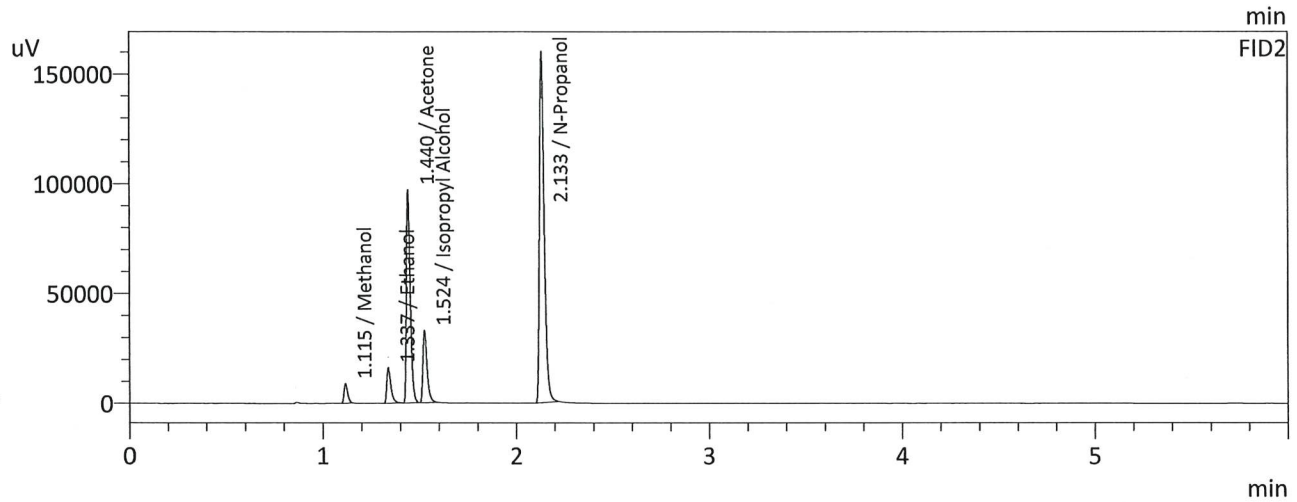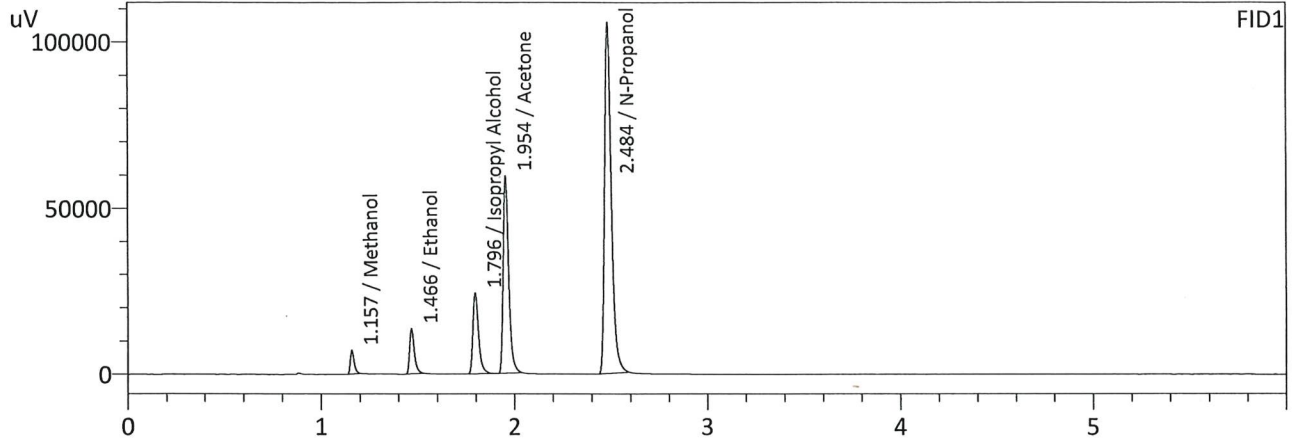

FID1



Name	Conc.	Area	Unit
Methanol	1.0000	10059	g/100cc
Ethanol	0.0534	22395	g/100cc
Isopropyl Alcohol	1.0000	49132	g/100cc
Acetone	1.0000	117760	g/100cc
N-Propanol	0.0000	252038	g/100cc
Flour. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	1.0000	11542	g/100cc
Ethanol	0.0550	24077	g/100cc
Acetone	1.0000	131832	g/100cc
Isopropyl Alcohol	1.0000	50196	g/100cc
N-Propanol	0.0000	271972	g/100cc
Flour. Hydrocarbon(s)	--	--	g/100cc

99

Sample Name : INT STD BLK 2  
 Laboratory : Coeur d' Alene Lab  
 Injection Date : 4/8/2023 5:24:09 PM  
 Vial # : 3  
 Method Filename : Default Project - ALCOHOL.gcm  
 Instrument #GC/HS : C12255850700 / C12595700181

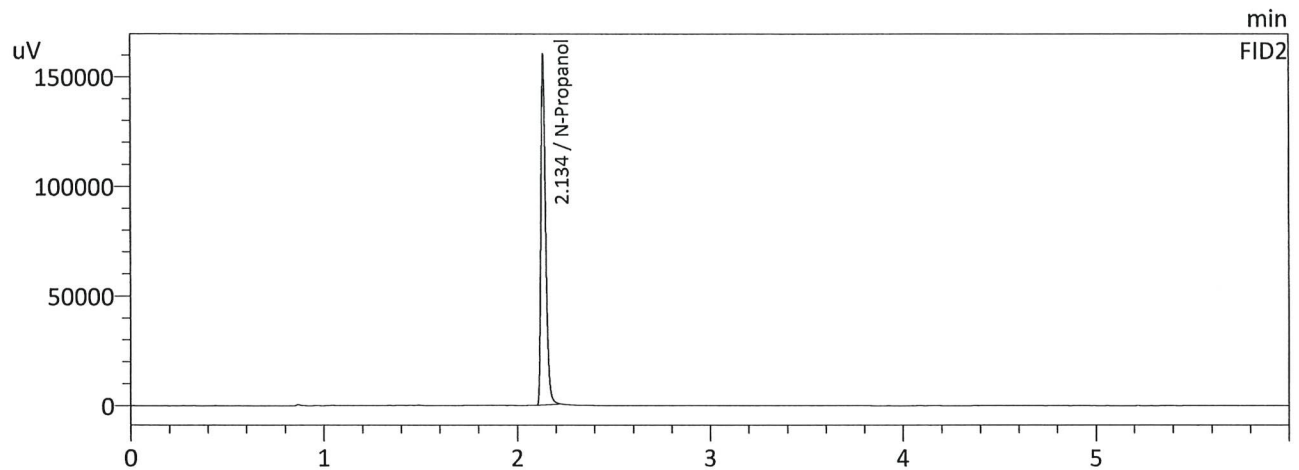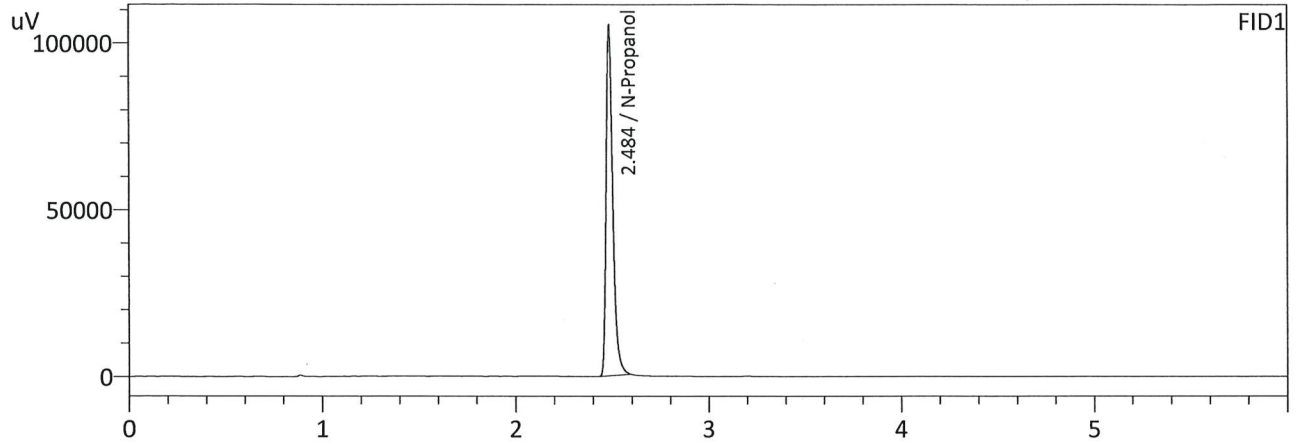

FID1

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	251615	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	--	--	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	272156	g/100cc
Flour. Hydrocarbon(s)	--	--	g/100cc

99

## VOLATILES DETERMINATION CASEFILE WORKSHEET

## VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No: QC-1-1

Analysis Date(s): 4/8/2023 5:32:48 PM(-07:00)

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Sample A-B Difference	Over-all Mean
Sample Results	0.0794	0.0796	0.0002	0.0795	0.0008	0.0799
(g/100cc)	0.0803	0.0803	0.0000	0.0803		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument information is stored centrally.

Refer To Instrument Method: ALCOHOL.gcm



Reporting of Results	Uncertainty of Measurements (UM%): 5.00%		
Overall Mean (g/100cc)	Low	High	5 % of Mean
0.079	0.075	0.083	0.004
	Reported Results		
	0.079		

Calibration and control data are stored centrally.



99

Sample Name : QC-1-1  
 Laboratory : Coeur d' Alene Lab  
 Injection Date : 4/8/2023 5:32:48 PM  
 Vial # : 4  
 Method Filename : Default Project - ALCOHOL.gcm  
 Instrument #GC/HS : C12255850700 / C12595700181

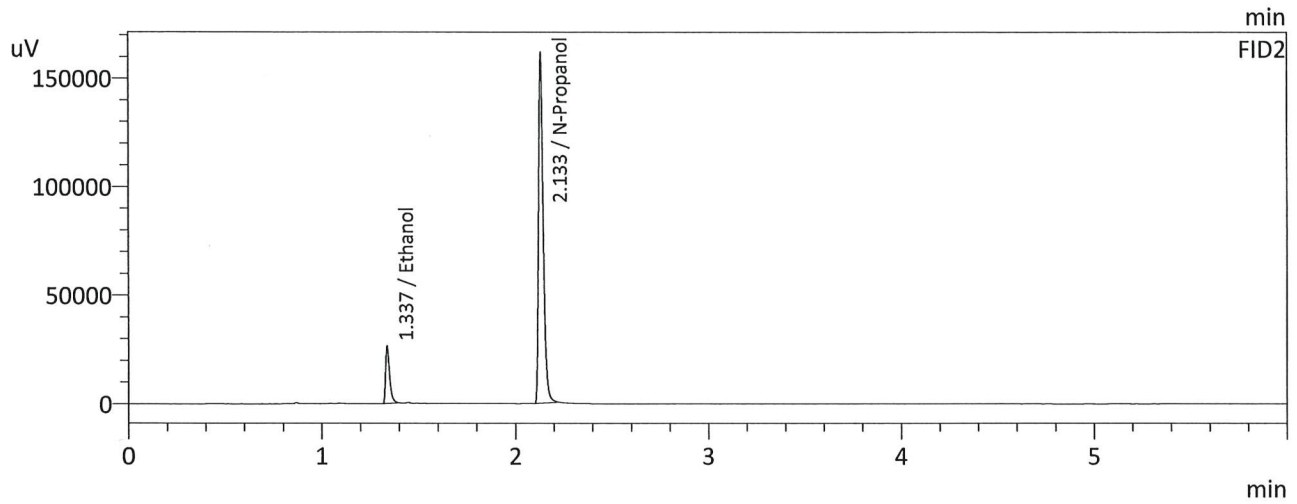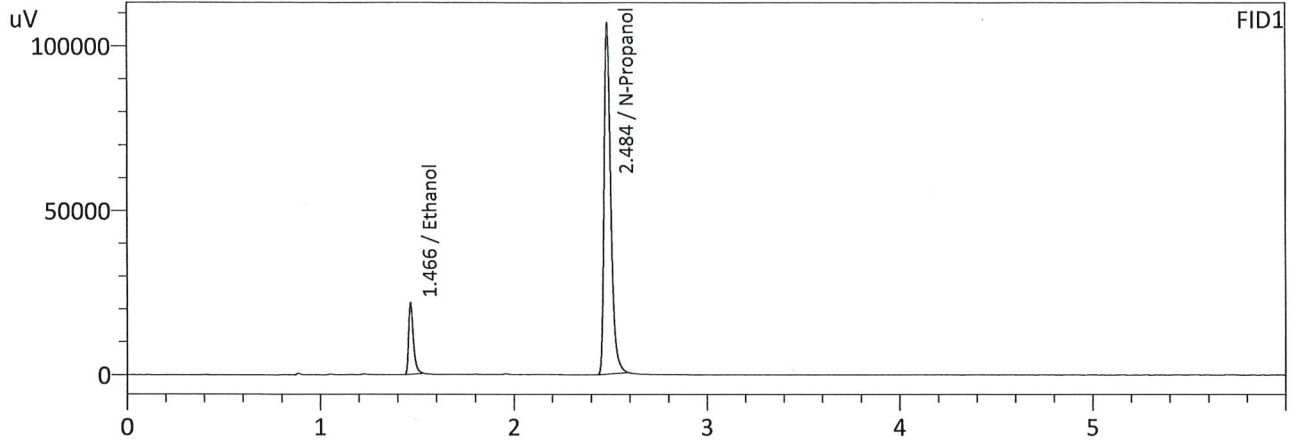

FID1



Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.0794	36023	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	254836	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.0796	38366	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	275225	g/100cc
Flour. Hydrocarbon(s)	--	--	g/100cc

99

Sample Name : QC-1-1-B  
 Laboratory : Coeur d' Alene Lab  
 Injection Date : 4/8/2023 5:43:31 PM  
 Vial # : 5  
 Method Filename : Default Project - ALCOHOL.gcm  
 Instrument #GC/HS : C12255850700 / C12595700181

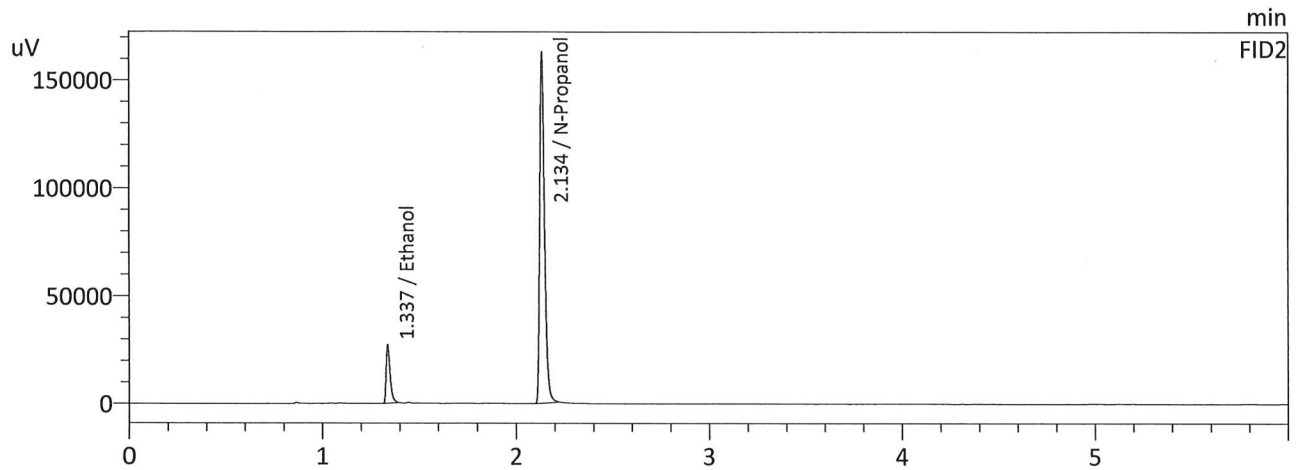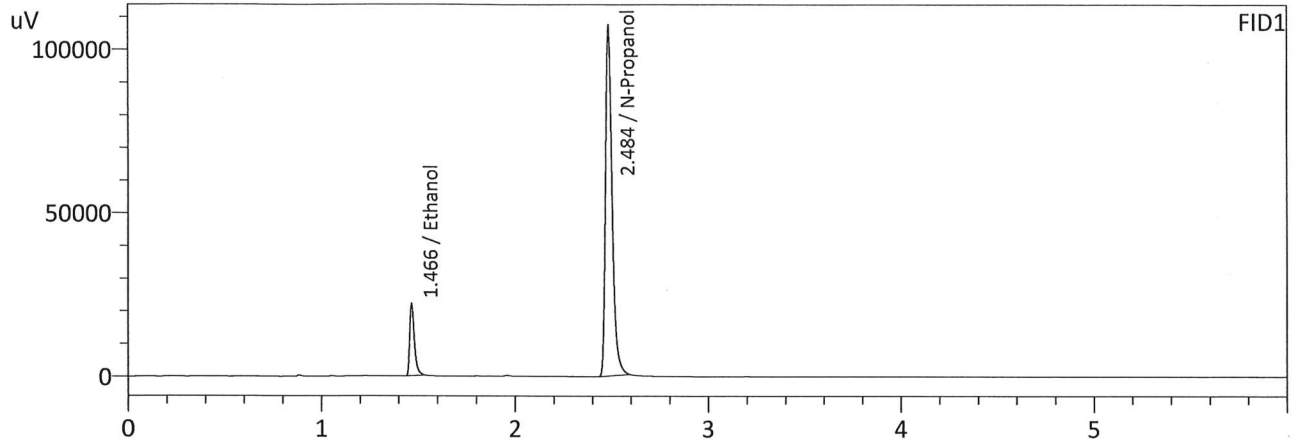

FID1

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.0803	36705	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	256196	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.0803	39077	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	277127	g/100cc
Flour. Hydrocarbon(s)	--	--	g/100cc

99

## VOLATILES DETERMINATION CASEFILE WORKSHEET

## VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No: QC-2-1

Analysis Date(s): 4/8/2023 5:52:11 PM(-07:00)

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Sample A-B Difference	Over-all Mean
Sample Results	0.1960	0.1949	0.0011	0.1954	0.0018	0.1963
(g/100cc)	0.1973	0.1971	0.0002	0.1972		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument information is stored centrally.



Refer To Instrument Method: ALCOHOL.gcm

Reporting of Results	Uncertainty of Measurements (UM%): 5.00%		
Overall Mean (g/100cc)	Low	High	5 % of Mean
0.196	0.186	0.206	0.010
	Reported Results		
	0.196		

Calibration and control data are stored centrally.

99

Sample Name : QC-2-1  
 Laboratory : Coeur d' Alene Lab  
 Injection Date : 4/8/2023 5:52:11 PM  
 Vial # : 6  
 Method Filename : Default Project - ALCOHOL.gcm  
 Instrument #GC/HS : C12255850700 / C12595700181

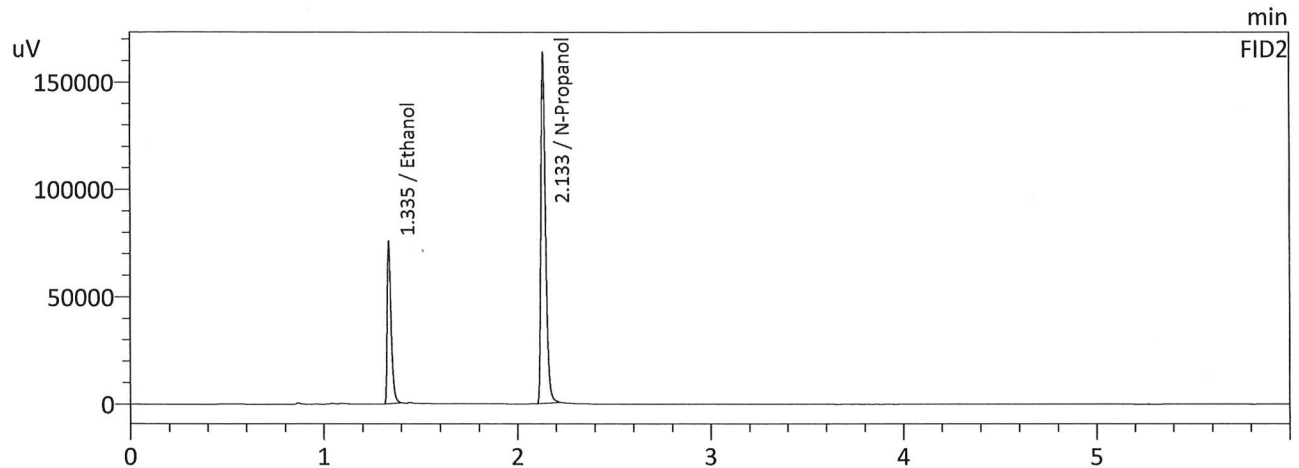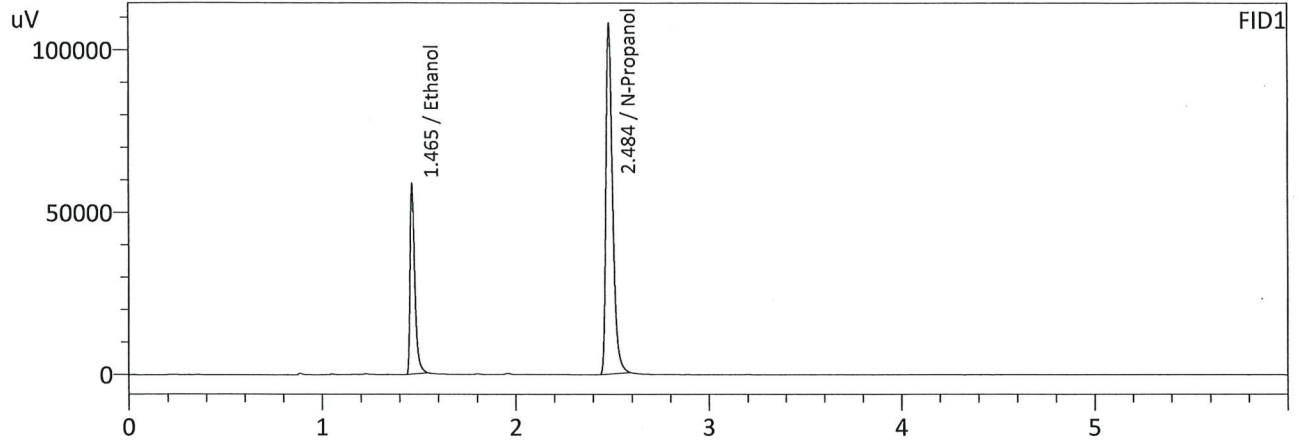

FID1

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.1960	97259	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	257504	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc



FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.1949	105386	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	278396	g/100cc
Flour. Hydrocarbon(s)	--	--	g/100cc



99

Sample Name : QC-2-1-B  
 Laboratory : Coeur d' Alene Lab  
 Injection Date : 4/8/2023 6:02:56 PM  
 Vial # : 7  
 Method Filename : Default Project - ALCOHOL.gcm  
 Instrument #GC/HS : C12255850700 / C12595700181

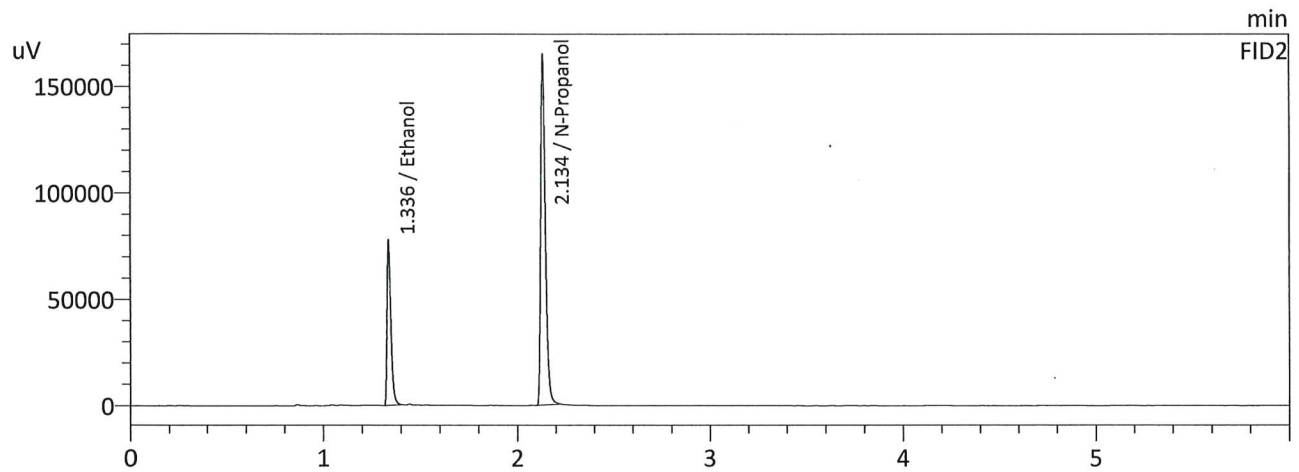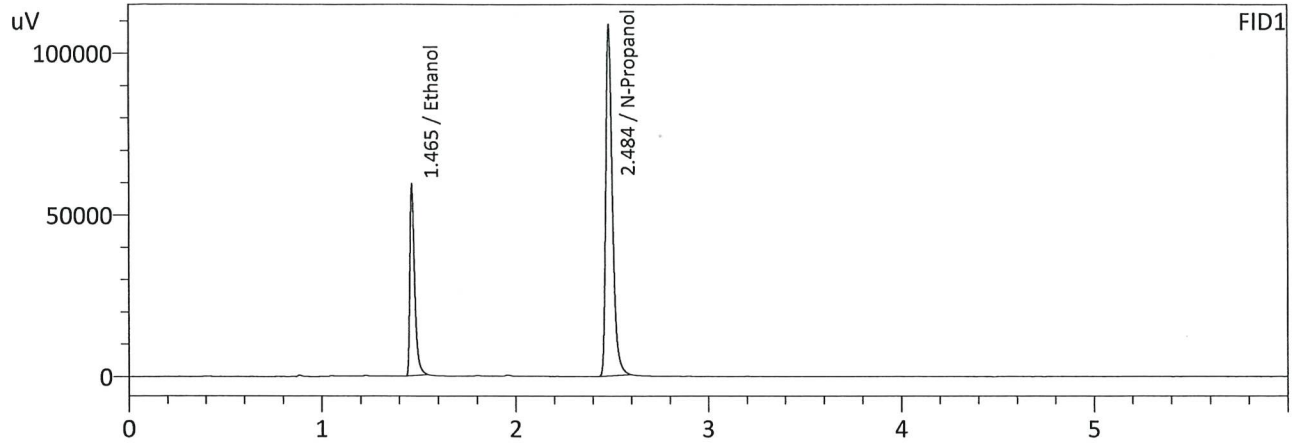

FID1

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.1973	98697	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	259613	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.1971	107443	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	280443	g/100cc
Flour. Hydrocarbon(s)	--	--	g/100cc

99

## VOLATILES DETERMINATION CASEFILE WORKSHEET

## VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No: 0.08 QA

Analysis Date(s): 4/8/2023 6:11:36 PM(-07:00)

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Sample A-B Difference	Over-all Mean
Sample Results	0.0823	0.0823	0.0000	0.0823	0.0004	0.0825
(g/100cc)	0.0828	0.0827	0.0001	0.0827		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument information is stored centrally.

Refer To Instrument Method: ALCOHOL.gcm



Reporting of Results	Uncertainty of Measurements (UM%): 5.00%		
Overall Mean (g/100cc)	Low	High	5 % of Mean
0.082	0.077	0.087	0.005

Reported Results	
0.082	

Calibration and control data are stored centrally.

99

Sample Name : 0.08 QA  
 Laboratory : Coeur d' Alene Lab  
 Injection Date : 4/8/2023 6:11:36 PM  
 Vial # : 8  
 Method Filename : Default Project - ALCOHOL.gcm  
 Instrument #GC/HS : C12255850700 / C12595700181

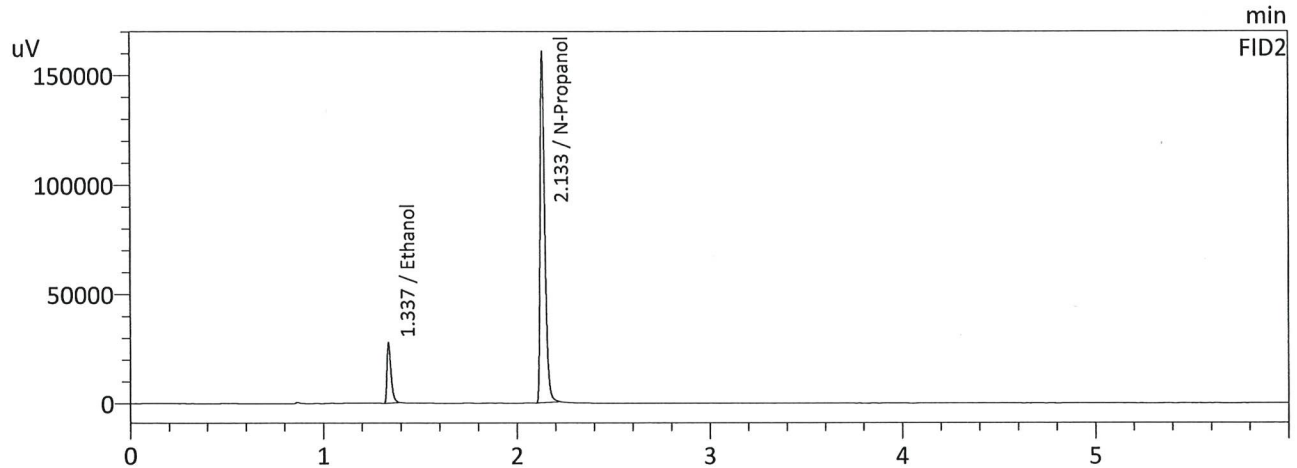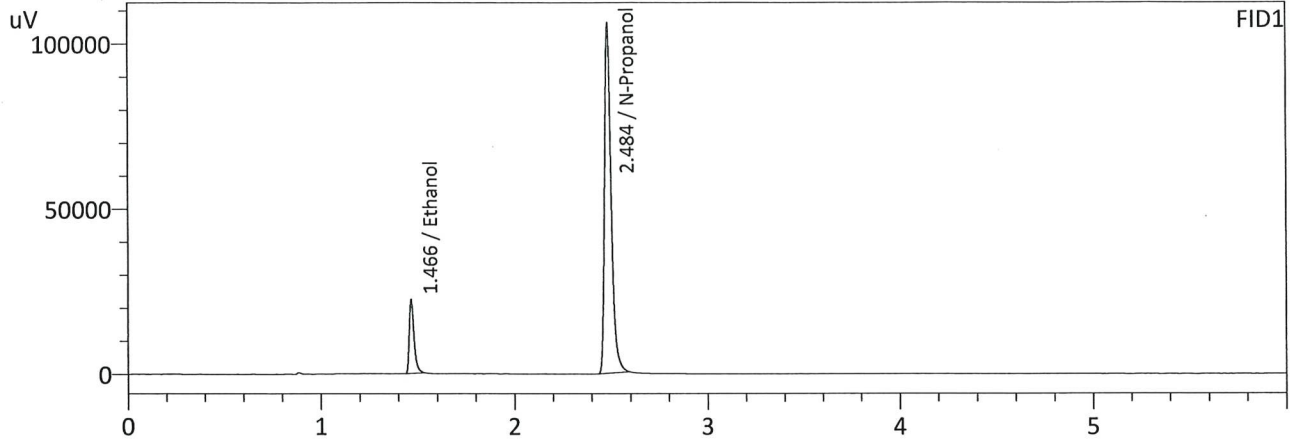

FID1



Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.0823	37239	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	252836	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.0823	39655	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	273488	g/100cc
Flour. Hydrocarbon(s)	--	--	g/100cc

99

Sample Name : 0.08 QA - B  
 Laboratory : Coeur d' Alene Lab  
 Injection Date : 4/8/2023 6:22:22 PM  
 Vial # : 9  
 Method Filename : Default Project - ALCOHOL.gcm  
 Instrument #GC/HS : C12255850700 / C12595700181

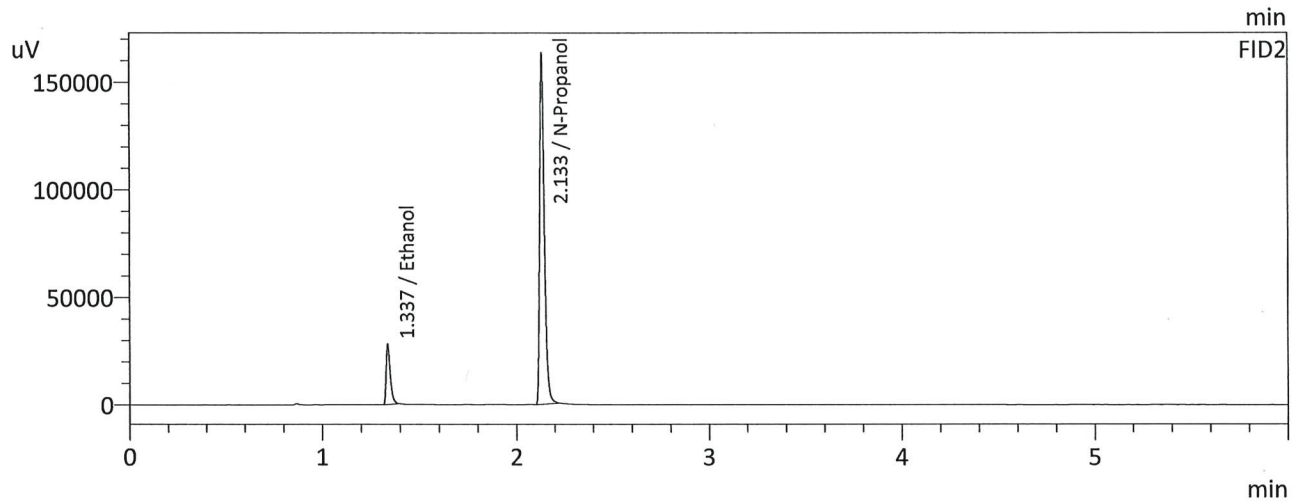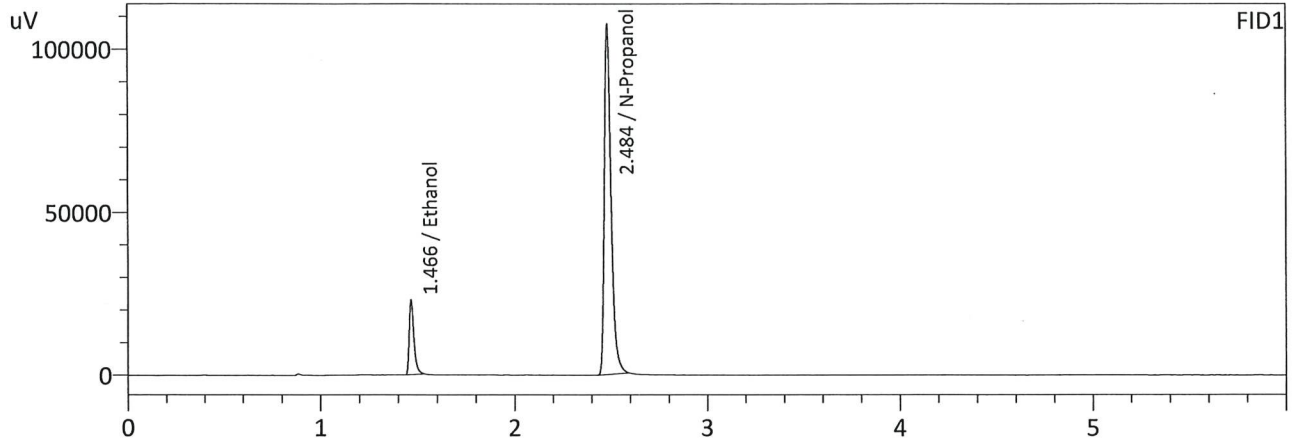

FID1

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.0828	37981	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	256221	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.0827	40459	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	277304	g/100cc
Flour. Hydrocarbon(s)	--	--	g/100cc



99

## VOLATILES DETERMINATION CASEFILE WORKSHEET

## VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No: QC-1-2

Analysis Date(s): 4/8/2023 9:06:13 PM(-07:00)

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Sample A-B Difference	Over-all Mean
Sample Results	0.0823	0.0823	0.0000	0.0823	0.0002	0.0822
(g/100cc)	0.0820	0.0822	0.0002	0.0821		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument information is stored centrally.



Refer To Instrument Method: ALCOHOL.gcm

Reporting of Results	Uncertainty of Measurements (UM%): 5.00%		
Overall Mean (g/100cc)	Low	High	5 % of Mean
0.082	0.077	0.087	0.005
	Reported Results		
	0.082		

Calibration and control data are stored centrally.

99

Sample Name : QC-1-2  
 Laboratory : Coeur d' Alene Lab  
 Injection Date : 4/8/2023 9:06:13 PM  
 Vial # : 26  
 Method Filename : Default Project - ALCOHOL.gcm  
 Instrument #GC/HS : C12255850700 / C12595700181

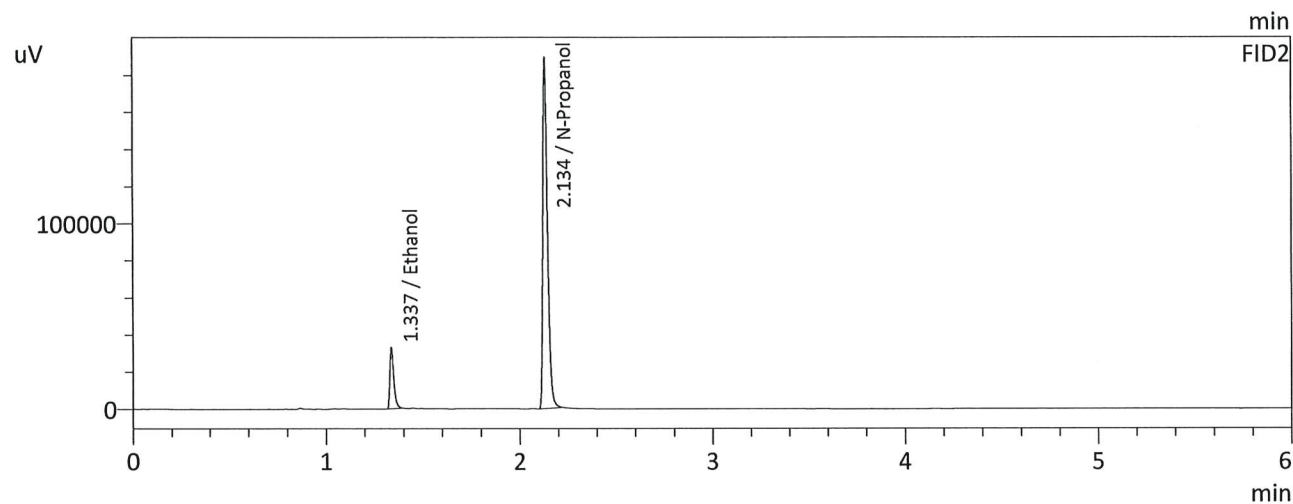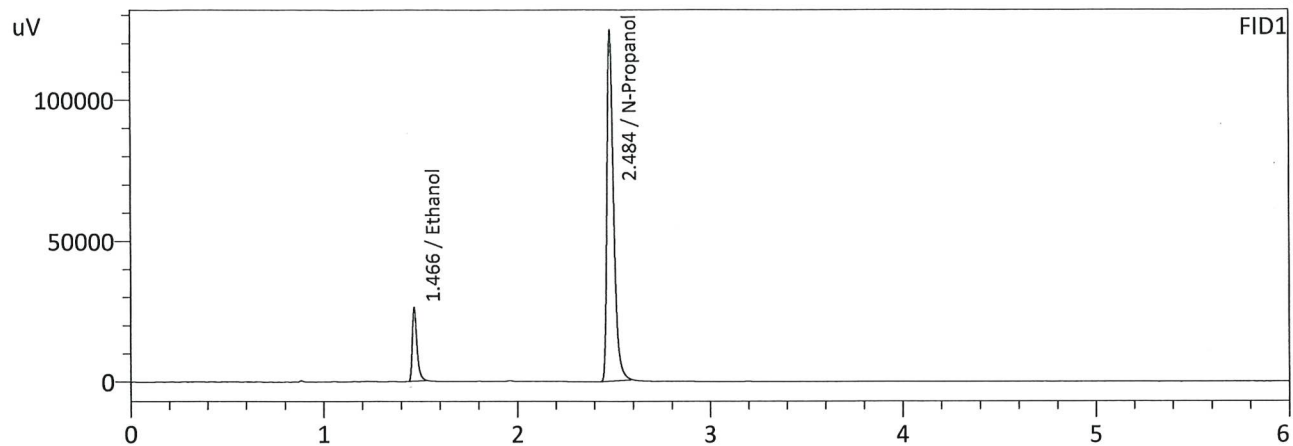

FID1



Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.0823	43740	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	297068	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.0823	46567	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	321152	g/100cc
Flour. Hydrocarbon(s)	--	--	g/100cc

99

Sample Name : QC-1-2-B  
 Laboratory : Coeur d' Alene Lab  
 Injection Date : 4/8/2023 9:16:56 PM  
 Vial # : 27  
 Method Filename : Default Project - ALCOHOL.gcm  
 Instrument #GC/HS : C12255850700 / C12595700181

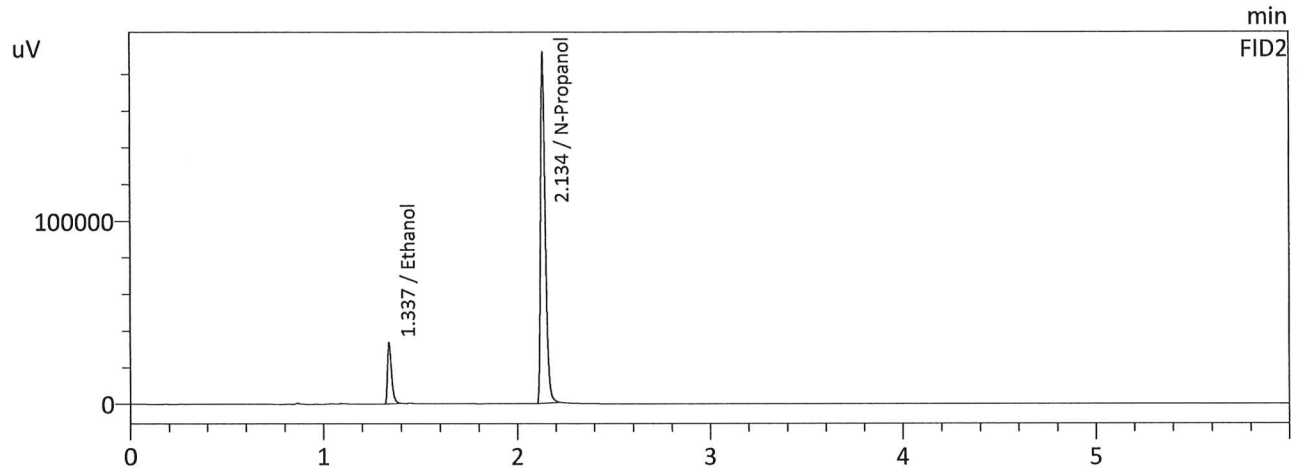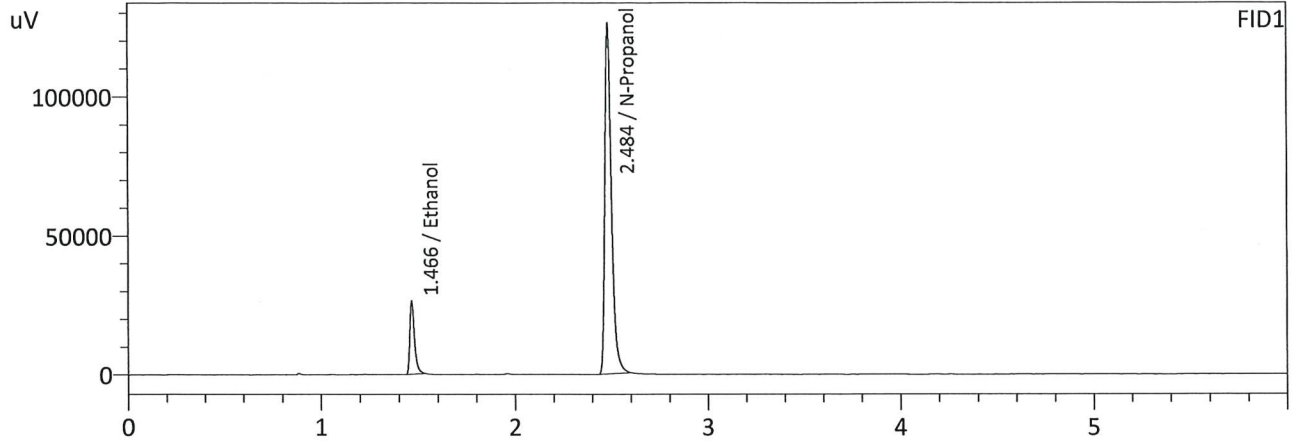

FID1

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.0820	44080	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	300413	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.0822	47059	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	324789	g/100cc
Flour. Hydrocarbon(s)	--	--	g/100cc

99

## VOLATILES DETERMINATION CASEFILE WORKSHEET

## VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No: QC-2-2

Analysis Date(s): 4/8/2023 9:25:36 PM(-07:00)

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Sample A-B Difference	Over-all Mean
Sample Results	0.2038	0.2032	0.0006	0.2035	0.0006	0.2032
(g/100cc)	0.2030	0.2029	0.0001	0.2029		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument information is stored centrally.



Refer To Instrument Method: ALCOHOL.gcm

Reporting of Results	Uncertainty of Measurements (UM%): 5.00%		
Overall Mean (g/100cc)	Low	High	5 % of Mean
0.203	0.192	0.214	0.011
	<b>Reported Results</b>		
	0.203		

Calibration and control data are stored centrally.

99

Sample Name : QC-2-2  
 Laboratory : Coeur d' Alene Lab  
 Injection Date : 4/8/2023 9:25:36 PM  
 Vial # : 28  
 Method Filename : Default Project - ALCOHOL.gcm  
 Instrument #GC/HS : C12255850700 / C12595700181

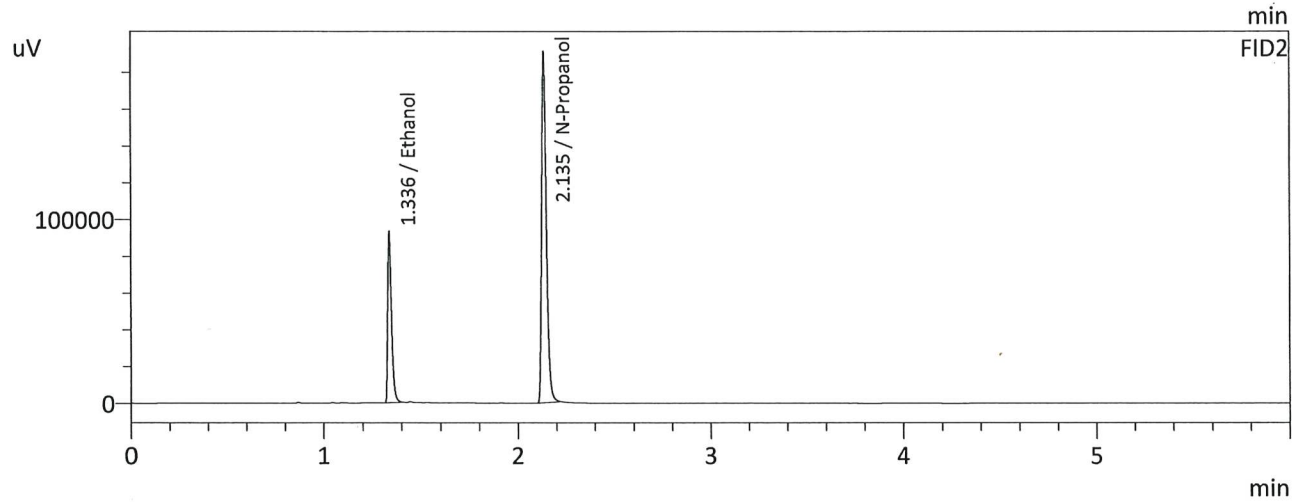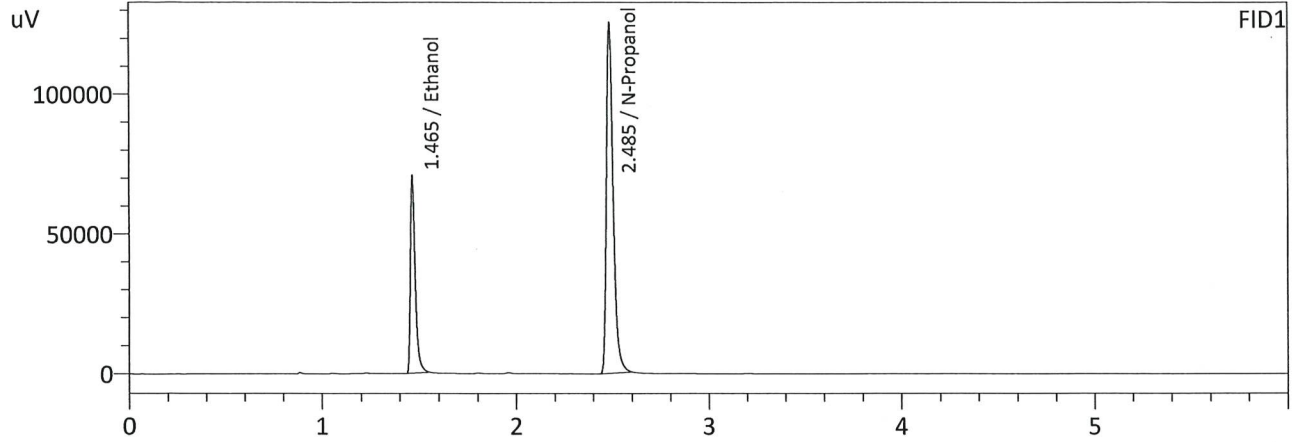

FID1

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.2038	117753	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	299319	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc



FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.2032	128114	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	323661	g/100cc
Flour. Hydrocarbon(s)	--	--	g/100cc



99

Sample Name : QC-2-2-B  
 Laboratory : Coeur d' Alene Lab  
 Injection Date : 4/8/2023 9:36:21 PM  
 Vial # : 29  
 Method Filename : Default Project - ALCOHOL.gcm  
 Instrument #GC/HS : C12255850700 / C12595700181

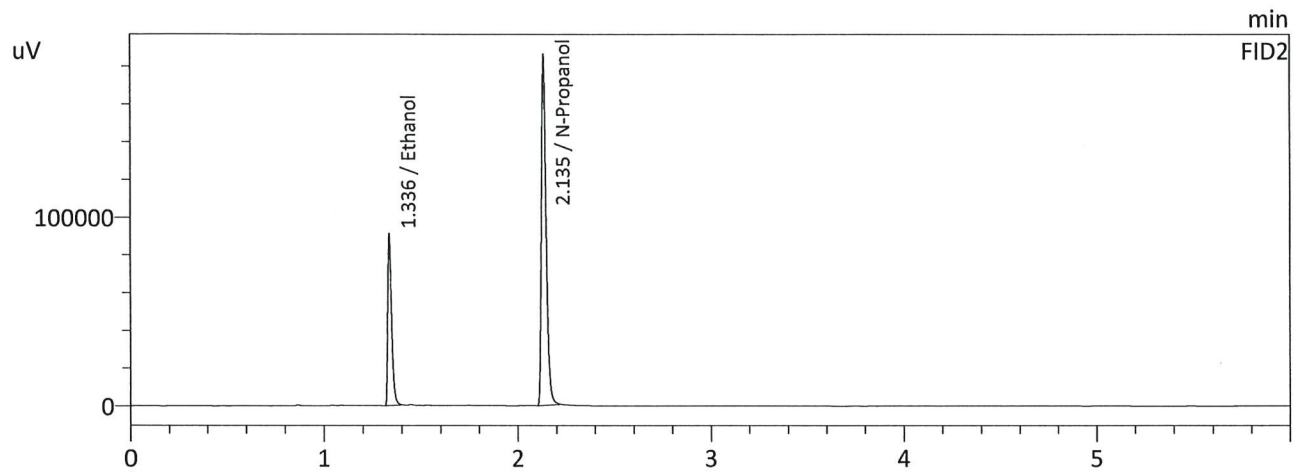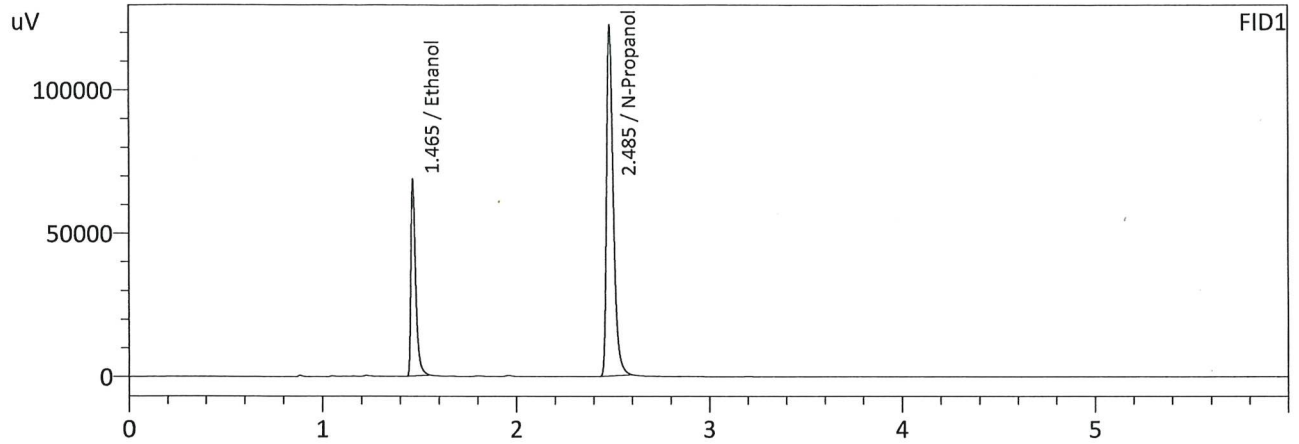

FID1



Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.2030	114417	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	292099	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	0.2029	124723	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	315712	g/100cc
Flour. Hydrocarbon(s)	--	--	g/100cc

99

Sample Name : INT STD BLK 3  
 Laboratory : Coeur d' Alene Lab  
 Injection Date : 4/8/2023 9:45:00 PM  
 Vial # : 30  
 Method Filename : Default Project - ALCOHOL.gcm  
 Instrument #GC/HS : C12255850700 / C12595700181

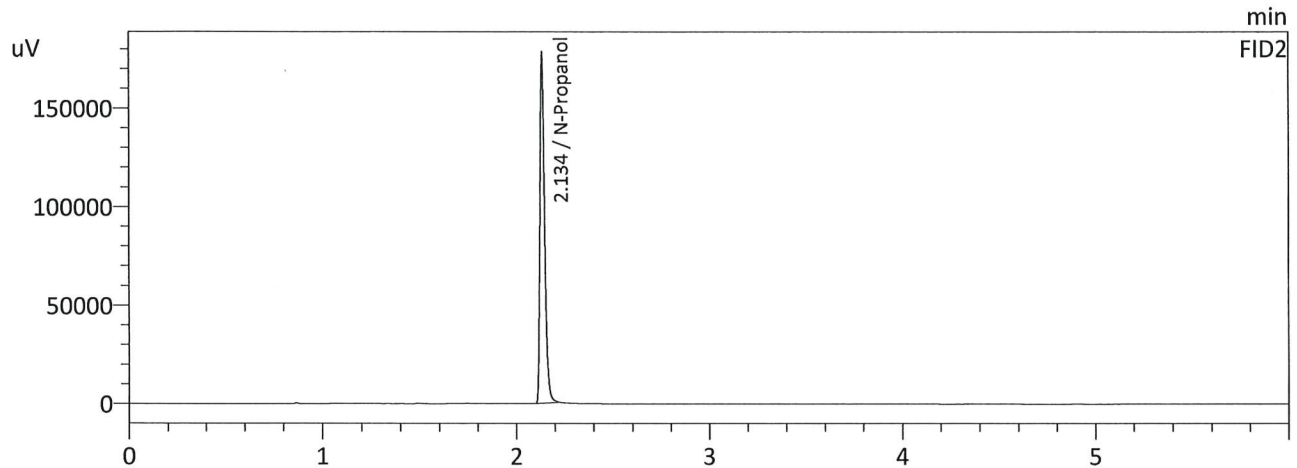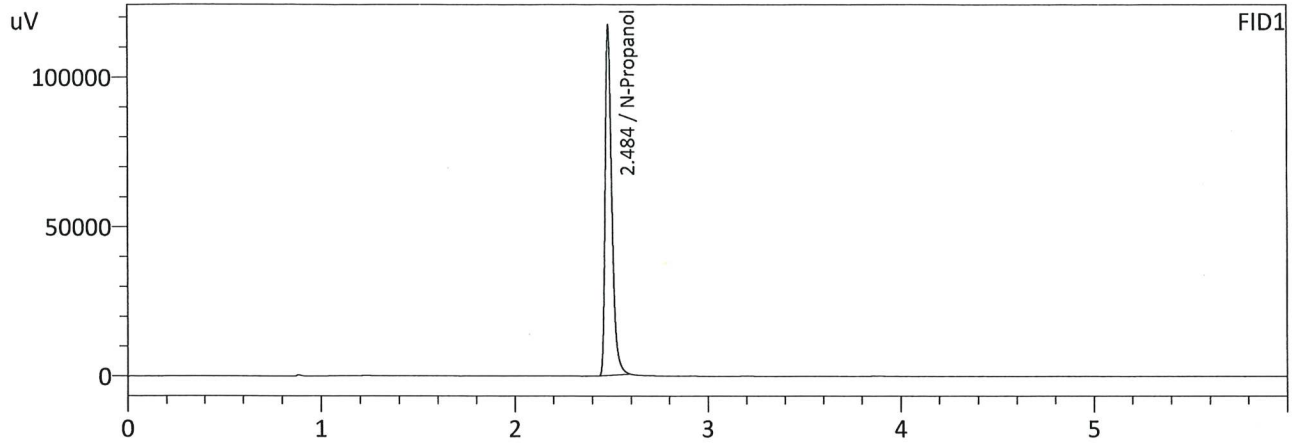

FID1



Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	279564	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	--	--	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	301740	g/100cc
Flour. Hydrocarbon(s)	--	--	g/100cc

99

Sample Name : INT STD BLK 4  
 Laboratory : Coeur d' Alene Lab  
 Injection Date : 4/8/2023 9:55:37 PM  
 Vial # : 31  
 Method Filename : Default Project - ALCOHOL.gcm  
 Instrument #GC/HS : C12255850700 / C12595700181

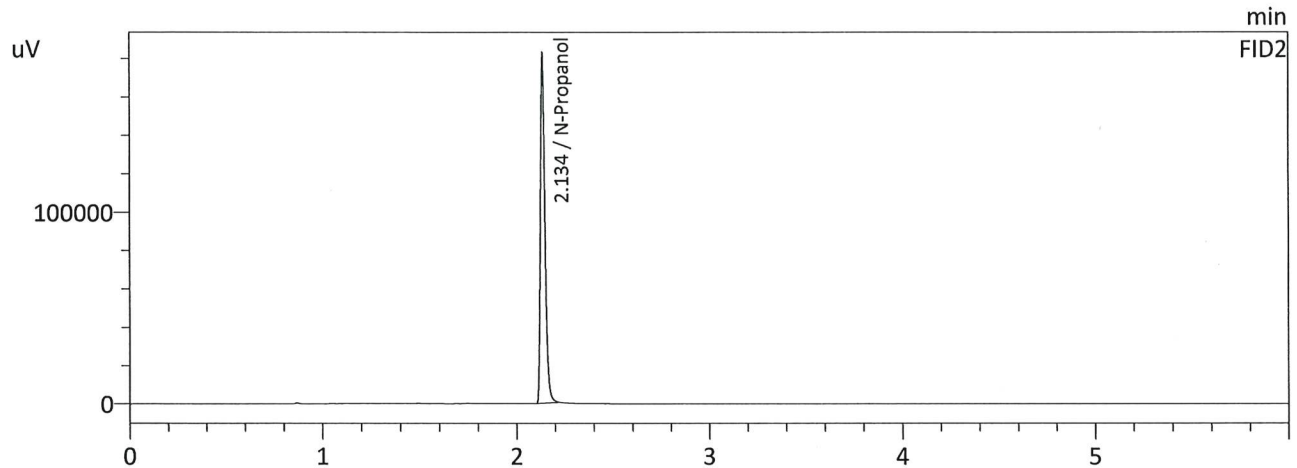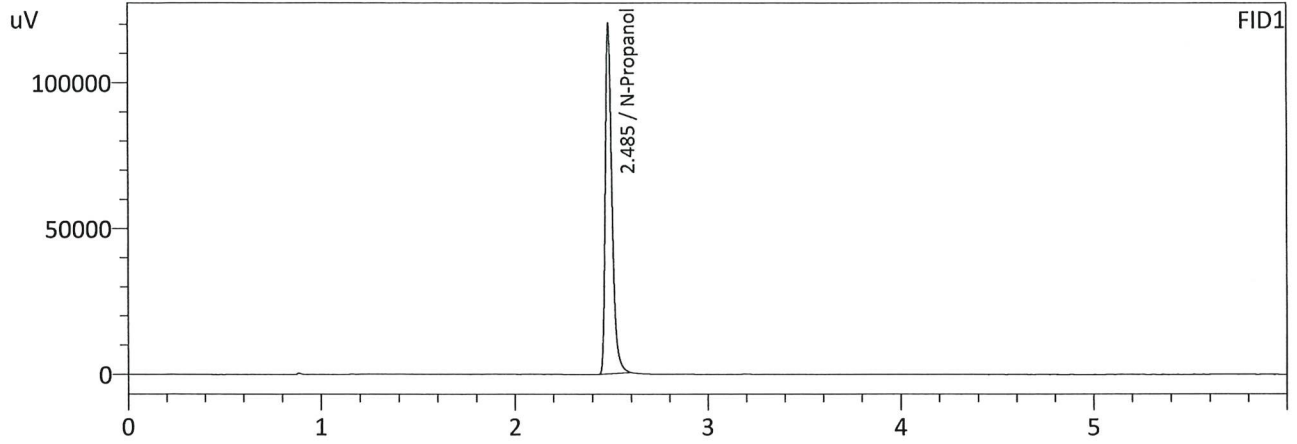

FID1

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
Acetone	--	--	g/100cc
N-Propanol	0.0000	286558	g/100cc
Fluor. Hydrocarbon(s)	--	--	g/100cc

FID2

Name	Conc.	Area	Unit
Methanol	--	--	g/100cc
Ethanol	--	--	g/100cc
Acetone	--	--	g/100cc
Isopropyl Alcohol	--	--	g/100cc
N-Propanol	0.0000	309615	g/100cc
Flour. Hydrocarbon(s)	--	--	g/100cc