Reviewed 1/19/17

1/18/2017

Worklist: 1496

LAB_CASE	ITEM	TASK_ID	DESCRIPTION
C2016-2132	1	72229	AM 8 Blood base neutral confir
C2016-2228	2	72251	AM 8 Blood base neutral confir
M2016-2783	2	72801	AM 8 Blood base neutral confir
M2016-2899	1	73028	AM 8 Blood base neutral confir
M2016-3601	1	73116	AM 8 Blood base neutral confir
M2016-4354	1	72991	AM 8 Blood base neutral confir
M2016-4868	1	72988	AM 8 Blood base neutral confir
P2016-1832	1	72923	AM 8 Blood base neutral confir
P2016-1837	1	72985	AM 8 Blood base neutral confir
P2016-1889	1	72211	AM 8 Blood base neutral confir
P2016-2086	1	72990	AM 8 Blood base neutral confir
P2016-2118	1	72119	AM 8 Blood base neutral confir
P2016-2119	1	72228	AM 8 Blood base neutral confir
P2016-2143	1	72118	AM 8 Blood base neutral confir
P2016-2356	1	73115	AM 8 Blood base neutral confir
P2016-2386	1	72984	AM 8 Blood base neutral confir
P2016-2426	1	72989	AM 8 Blood base neutral confir
P2016-2442	1	72232	AM 8 Blood base neutral confir
P2016-2486	1	72987	AM 8 Blood base neutral confir
P2016-2592	1	72231	AM 8 Blood base neutral confir
P2016-2634	1	72230	AM 8 Blood base neutral confir
P2016-2665	1	73318	AM 8 Blood base neutral confir
P2016-2733	1	72996	AM 8 Blood base neutral confir

Worklist: 1496

LAB_CASE	ITEM	TASK_ID	DESCRIPTION
P2016-2826	3	72997	AM 8 Blood base neutral confir
P2016-2834	1	72986	AM 8 Blood base neutral confir

Sequence verified 1/18/17 JM

JM

simulate_sequence.log

Simulate Run Sequence Fri Jan 13 15:31:58 2017

Instrument Name: Major Mass Spec
Sequence File: D:\MassHunter\GCMS\1\sequence\RMs.sequence.xml
Comment: MassHunter sequence
Operator: ISP\datastor
Data Path: D:\DATA\TM\2017\01132017\
Method Path: D:\MassHunter\GCMS\1\METHODS\

Line	Type	Vials	DataFile	Sample Name
Acquisition Method: BNSB120510.M				
1)	Sample	100	Prerun Solvent Blank	Pre-run Solvent Blank
2)	Sample	1 ✓	Negative Control-BN	Negative Control - ...1013
3)	Sample	2 ✓	Spiked Positive Control-BN	Positive Control
4)	Sample	99	prbLK2	Solvent Blank
Acquisition Method: GBT092509-Delta EMV.M				
5)	Sample	100	Prerun Solvent Blankr	Pre-run Solvent Blank
6)	Sample	1 ✓	Negative Control-BNr	Negative Control - ...1013
7)	Sample	2 ✓	Spiked Positive Control-BNr	Positive Control
8)	Sample	99	prbLK2r	Solvent Blank
Acquisition Method: BNSB120510.M				
9)	Sample	100	C2016-2132-1-BNBLK	Lab No.: C2016-2132-1
10)	Sample	3 ✓	C2016-2132-1-BN	Lab No.: C2016-2132-1
Acquisition Method: GBT092509-Delta EMV.M				
11)	Sample	3 ✓	C2016-2132-1-BNr	Lab No.: C2016-2132-1
Acquisition Method: BNSB120510.M				
12)	Sample	100	C2016-2228-2-BNBLK	Lab No.: C2016-2228-2
13)	Sample	4 ✓	C2016-2228-2-BN	Lab No.: C2016-2228-2
Acquisition Method: GBT092509-Delta EMV.M				
14)	Sample	4 ✓	C2016-2228-2-BNr	Lab No.: C2016-2228-2
Acquisition Method: BNSB120510.M				
15)	Sample	100	M2016-2783-2-BNBLK	Lab No.: M2016-2783-2
16)	Sample	5 ✓	M2016-2783-2-BN	Lab No.: M2016-2783-2
Acquisition Method: GBT092509-Delta EMV.M				
17)	Sample	5 ✓	M2016-2783-2-BNr	Lab No.: M2016-2783-2
Acquisition Method: BNSB120510.M				
18)	Sample	100 ✓	M2016-2899-1-BNBLK	Lab No.: M2016-2899-1
19)	Sample	6	M2016-2899-1-BN	Lab No.: M2016-2899-1
Acquisition Method: GBT092509-Delta EMV.M				
20)	Sample	6 ✓	M2016-2899-1-BNr	Lab No.: M2016-2899-1
Acquisition Method: BNSB120510.M				
21)	Sample	100 ✓	M2016-3601-1-BNBLK	Lab No.: M2016-3601-1
22)	Sample	7	M2016-3601-1-BN	Lab No.: M2016-3601-1
Acquisition Method: GBT092509-Delta EMV.M				
23)	Sample	7 ✓	M2016-3601-1-BNr	Lab No.: M2016-3601-1
Acquisition Method: BNSB120510.M				
24)	Sample	100 ✓	M2016-4354-1-BNBLK	Lab No.: M2016-4354-1
25)	Sample	8	M2016-4354-1-BN	Lab No.: M2016-4354-1
Acquisition Method: GBT092509-Delta EMV.M				
26)	Sample	8 ✓	M2016-4354-1-BNr	Lab No.: M2016-4354-1

```
Acquisition Method: BNSB120510.M
 27) Sample        100      M2016-4868-1-BNBLK     Lab No.:  M2016-4868-1
 28) Sample         9       M2016-4868-1-BN        Lab No.:  M2016-4868-1

Acquisition Method: GBT092509-Delta EMV.M
 29) Sample         9       M2016-4868-1-BNr       Lab No.:  M2016-4868-1

Acquisition Method: BNSB120510.M
 30) Sample        100      P2016-1832-1-BNBLK     Lab No.:  P2016-1832-1
 31) Sample         10      P2016-1832-1-BN        Lab No.: P2016-1832-1

Acquisition Method: GBT092509-Delta EMV.M
 32) Sample         10      P2016-1832-1-BNr       Lab No.:  P2016-1832-1

Acquisition Method: BNSB120510.M
 33) Sample        100      P2016-1837-1-BNBLK     Lab No.:  P2016-1837-1
 34) Sample         11      P2016-1837-1-BN        Lab No.:  P2016-1837-1

Acquisition Method: GBT092509-Delta EMV.M
 35) Sample         11      P2016-1837-1-BNr       Lab No.:  P2016-1837-1

Acquisition Method: BNSB120510.M
 36) Sample        100      P2016-1889-1-BNBLK     Lab No.:  P2016-1889-1
 37) Sample         12      P2016-1889-1-BN        Lab No.:  P2016-1889-1

Acquisition Method: GBT092509-Delta EMV.M
 38) Sample         12      P2016-1889-1-BNr       Lab No.:  P2016-1889-1

Acquisition Method: BNSB120510.M
 39) Sample        100      P2016-2086-1-BNBLK     Lab No.:  P2016-2086-1
 40) Sample         13      P2016-2086-1-BN        Lab No.:  P2016-2086-1

Acquisition Method: GBT092509-Delta EMV.M
 41) Sample         13      P2016-2086-1-BNr       Lab No.:  P2016-2086-1

Acquisition Method: BNSB120510.M
 42) Sample        100      P2016-2118-1-BNBLK     Lab No.:  P2016-2118-1
 43) Sample         14      P2016-2118-1-BN        Lab No.:  P2016-2118-1

Acquisition Method: GBT092509-Delta EMV.M
 44) Sample         14      P2016-2118-1-BNr       Lab No.:  P2016-2118-1

Acquisition Method: BNSB120510.M
 45) Sample        100      P2016-2119-1-BNBLK     Lab No.:  P2016-2119-1
 46) Sample         15      P2016-2119-1-BN        Lab No.:  P2016-2119-1

Acquisition Method: GBT092509-Delta EMV.M
 47) Sample         15      P2016-2119-1-BNr       Lab No.:  P2016-2119-1

Acquisition Method: BNSB120510.M
 48) Sample         99      P2016-2143-1-BNBLK     Lab No.:  P2016-2143-1
 49) Sample         16      P2016-2143-1-BN        Lab No.:  P2016-2143-1

Acquisition Method: GBT092509-Delta EMV.M
 50) Sample         16      P2016-2143-1-BNr       Lab No.:  P2016-2143-1

Acquisition Method: BNSB120510.M
 51) Sample         99      P2016-2356-1-BNBLK     Lab No.:  P2016-2356-1
 52) Sample         17      P2016-2356-1-BN        Lab No.:  P2016-2356-1

Acquisition Method: GBT092509-Delta EMV.M
 53) Sample         17      P2016-2356-1-BNr       Lab No.:  P2016-2356-1

Acquisition Method: BNSB120510.M
 54) Sample         99      P2016-2386-1-BNBLK     Lab No.:  P2016-2386-1
 55) Sample         18      P2016-2386-1-BN        Lab No.:  P2016-2386-1
```

```
Acquisition Method: GBT092509-Delta EMV.M
 56) Sample          18      P2016-2386-1-BNr        Lab No.:  P2016-2386-1

Acquisition Method: BNSB120510.M
 57) Sample          99      P2016-2426-1-BNBLK      Lab No.:  P2016-2426-1
 58) Sample          19      P2016-2426-1-BN         Lab No.:  P2016-2426-1

Acquisition Method: GBT092509-Delta EMV.M
 59) Sample          19      P2016-2426-1-BNr        Lab No.:  P2016-2426-1

Acquisition Method: BNSB120510.M
 60) Sample          99      P2016-2442-1-BNBLK      Lab No.:  P2016-2442-1
 61) Sample          20      P2016-2442-1-BN         Lab No.:  P2016-2442-1

Acquisition Method: GBT092509-Delta EMV.M
 62) Sample          20      P2016-2442-1-BNr        Lab No.:  P2016-2442-1

Acquisition Method: BNSB120510.M
 63) Sample          99      P2016-2486-1-BNBLK      Lab No.:  P2016-2486-1
 64) Sample          21      P2016-2486-1-BN         Lab No.:  P2016-2486-1

Acquisition Method: GBT092509-Delta EMV.M
 65) Sample          21      P2016-2486-1-BNr        Lab No.:  P2016-2486-1

Acquisition Method: BNSB120510.M
 66) Sample          99      P2016-2592-1-BNBLK      Lab No.:  P2016-2592-1
 67) Sample          22      P2016-2592-1-BN         Lab No.:  P2016-2592-1

Acquisition Method: GBT092509-Delta EMV.M
 68) Sample          22      P2016-2592-1-BNr        Lab No.:  P2016-2592-1

Acquisition Method: BNSB120510.M
 69) Sample          99      P2016-2634-1-BNBLK      Lab No.:  P2016-2634-1
 70) Sample          23      P2016-2634-1-BN         Lab No.:  P2016-2634-1

Acquisition Method: GBT092509-Delta EMV.M
 71) Sample          23      P2016-2634-1-BNr        Lab No.:  P2016-2634-1

Acquisition Method: BNSB120510.M
 72) Sample          99      P2016-2665-1-BNBLK      Lab No.:  P2016-2665-1
 73) Sample          24      P2016-2665-1-BN         Lab No.:  P2016-2665-1

Acquisition Method: GBT092509-Delta EMV.M
 74) Sample          24      P2016-2665-1-BNr        Lab No.:  P2016-2665-1

Acquisition Method: BNSB120510.M
 75) Sample          99      P2016-2733-1-BNBLK      Lab No.:  P2016-2733-1
 76) Sample          25      P2016-2733-1-BN         Lab No.:  P2016-2733-1

Acquisition Method: GBT092509-Delta EMV.M
 77) Sample          25      P2016-2733-1-BNr        Lab No.:  P2016-2733-1

Acquisition Method: BNSB120510.M
 78) Sample          99      P2016-2826-3-BNBLK      Lab No.:  P2016-2826-3
 79) Sample          26      P2016-2826-3-BN         Lab No.:  P2016-2826-3

Acquisition Method: GBT092509-Delta EMV.M
 80) Sample          26      P2016-2826-3-BNr        Lab No.:  P2016-2826-3

Acquisition Method: BNSB120510.M
 81) Sample          99      P2016-2834-1-BNBLK      Lab No.:  P2016-2834-1
 82) Sample          27      P2016-2834-1-BN         Lab No.:  P2016-2834-1

Acquisition Method: GBT092509-Delta EMV.M
 83) Sample          27      P2016-2834-1-BNr        Lab No.:  P2016-2834-1

Acquisition Method: BNSB120510.M
 84) Sample          99      POSTBLK                 BLK
```

simulate_sequence.log

```
Acquisition Method: GBT092509-Delta EMV.M
 85) Sample          99      AFTER                   BLK
megabytes Needed: 1362  Space on drive D: 198634
Sequence Verification Done!
```

File :I:\Instrument Data\Pocatello\Major Mass Spec\TM\2017\0113201
... 7\Negative Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 13 Jan 2017 16:04 using AcqMethod BNSB120510.M
Sample Name: Negative Control - Utak Lot B1013
Misc Info : Analytical Method 8

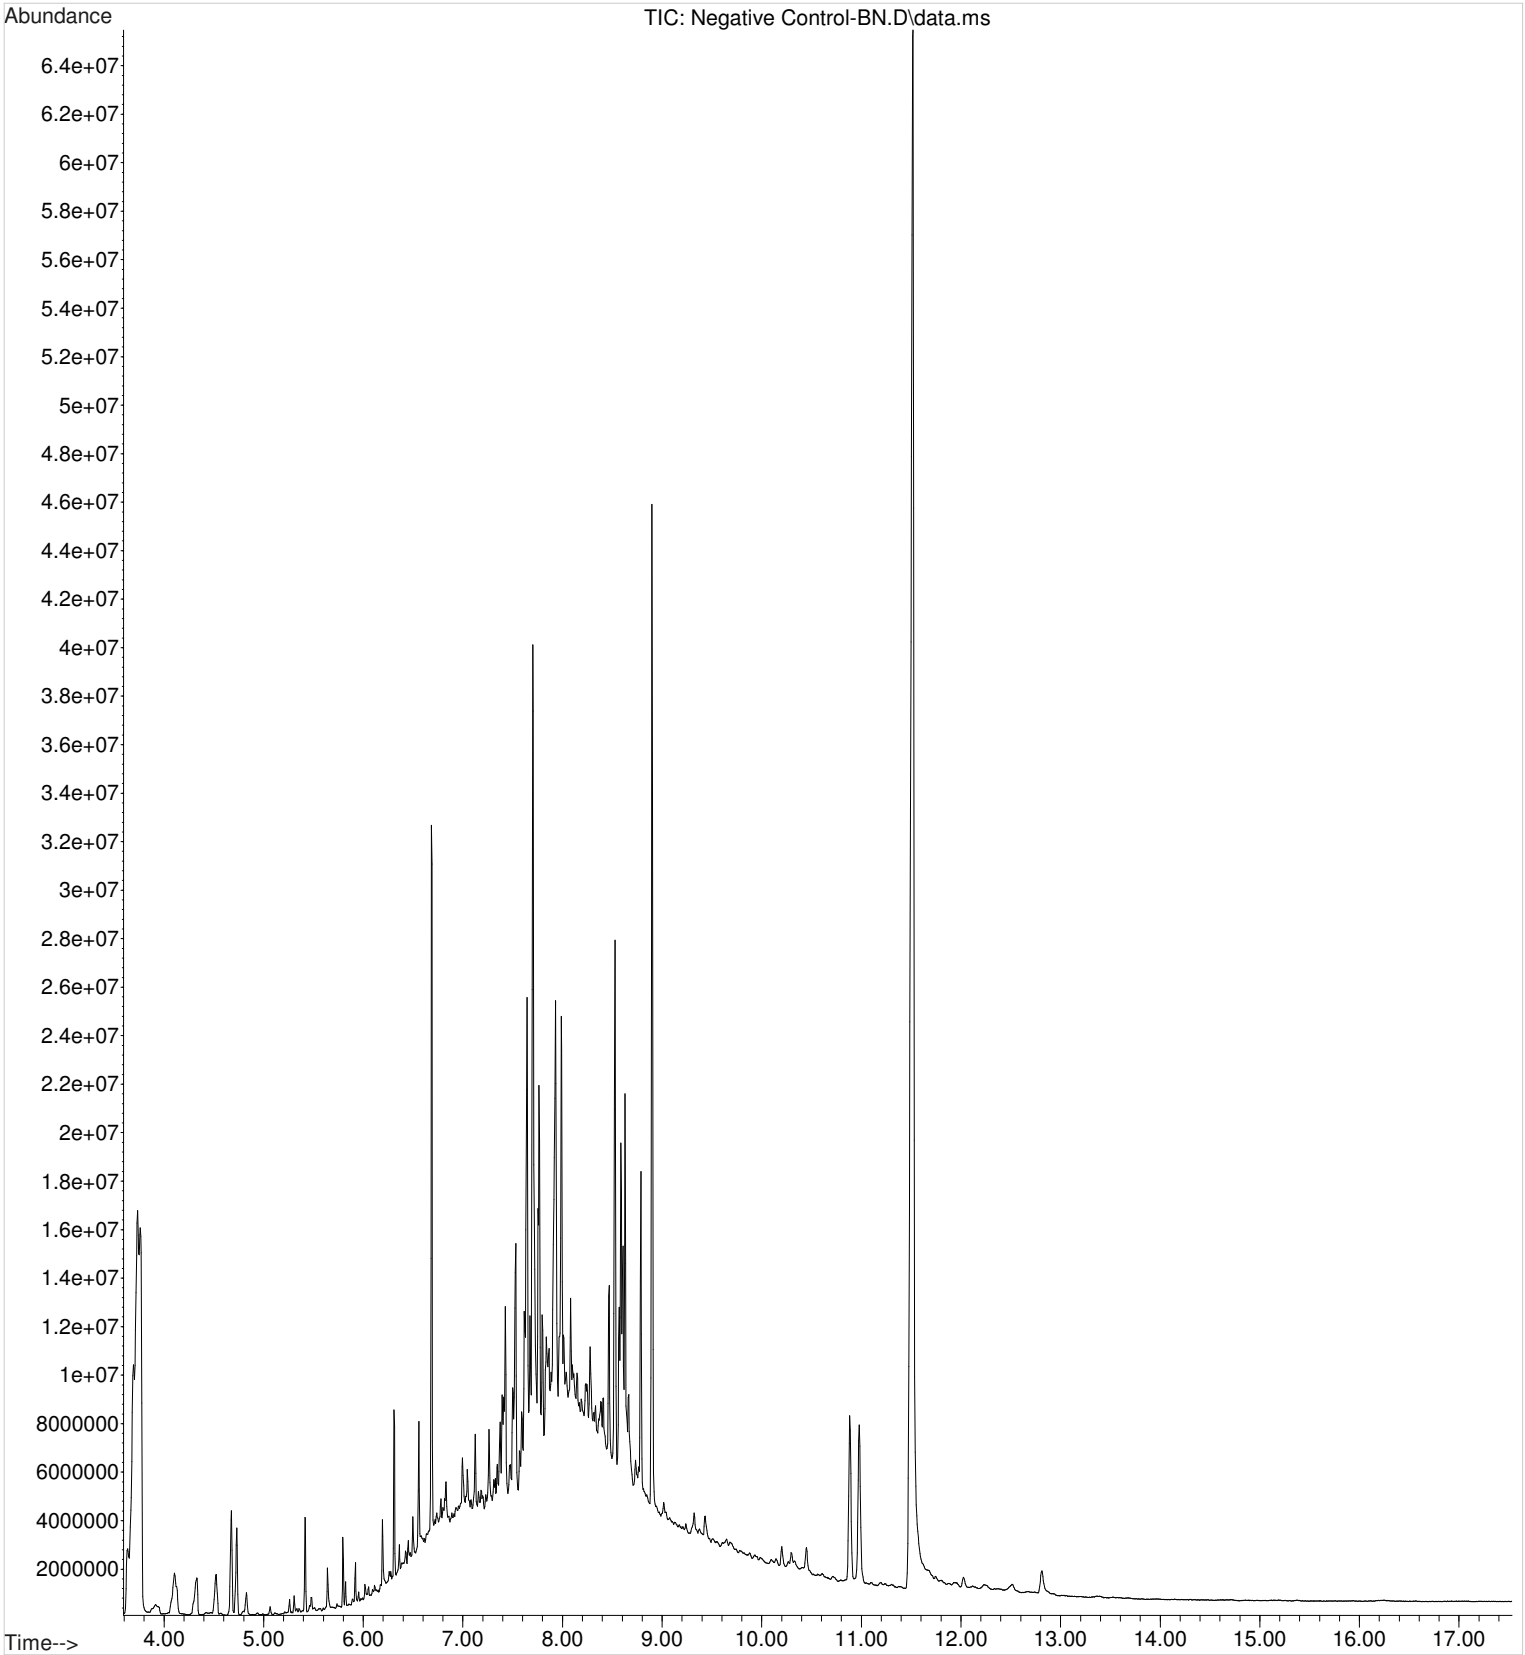

File :I:\Instrument Data\Pocatello\Major Mass Spec\TM\2017\0113201
... 7\Negative Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 13 Jan 2017 16:04 using AcqMethod BNSB120510.M
Sample Name: Negative Control - Utak Lot B1013
Misc Info : Analytical Method 8

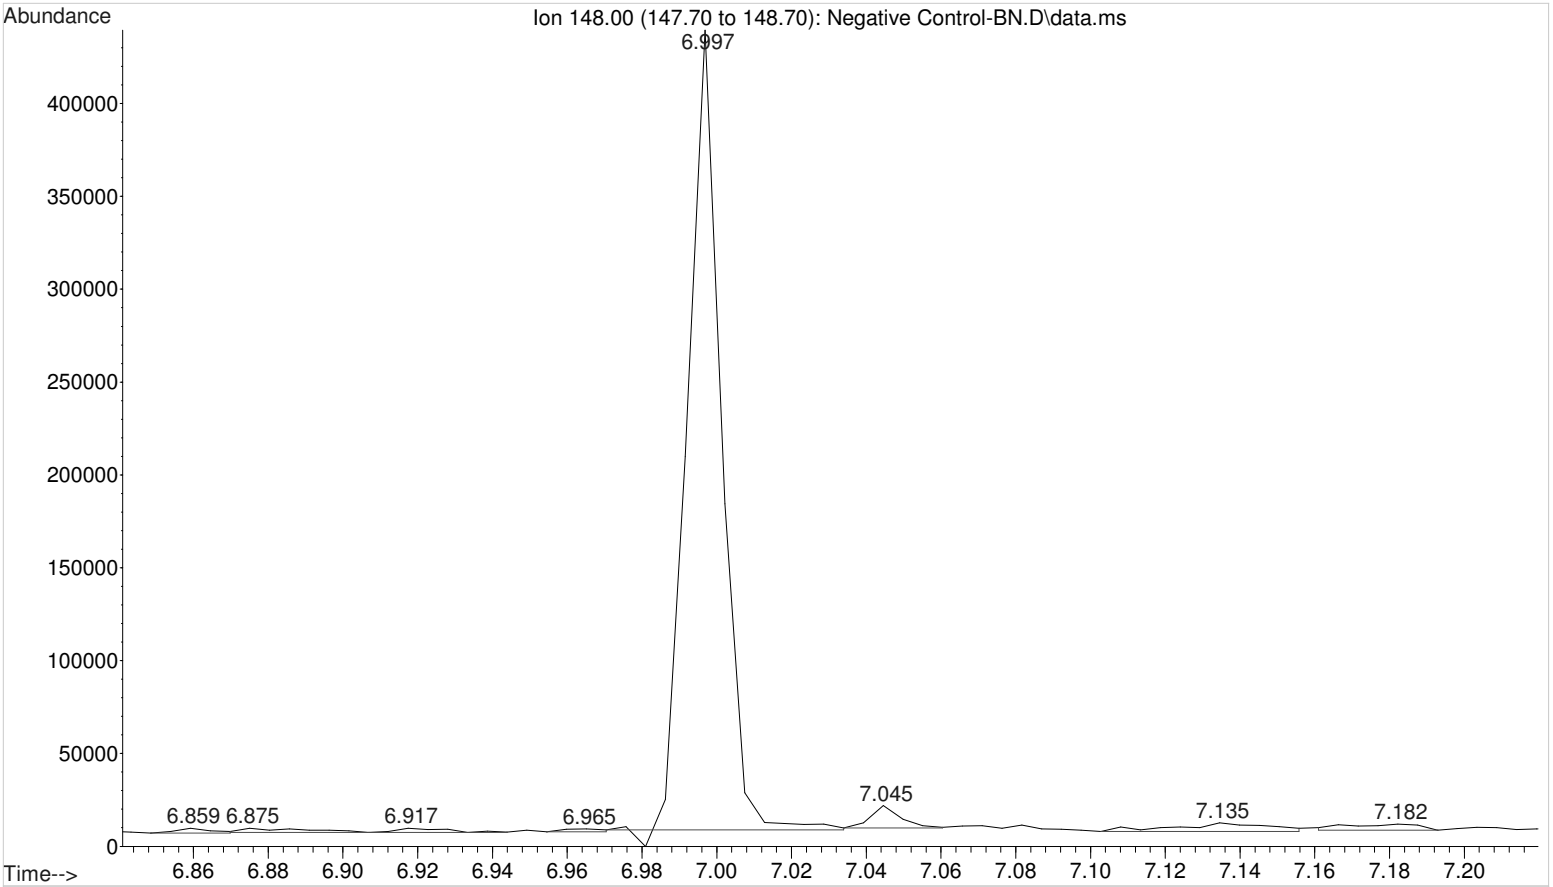

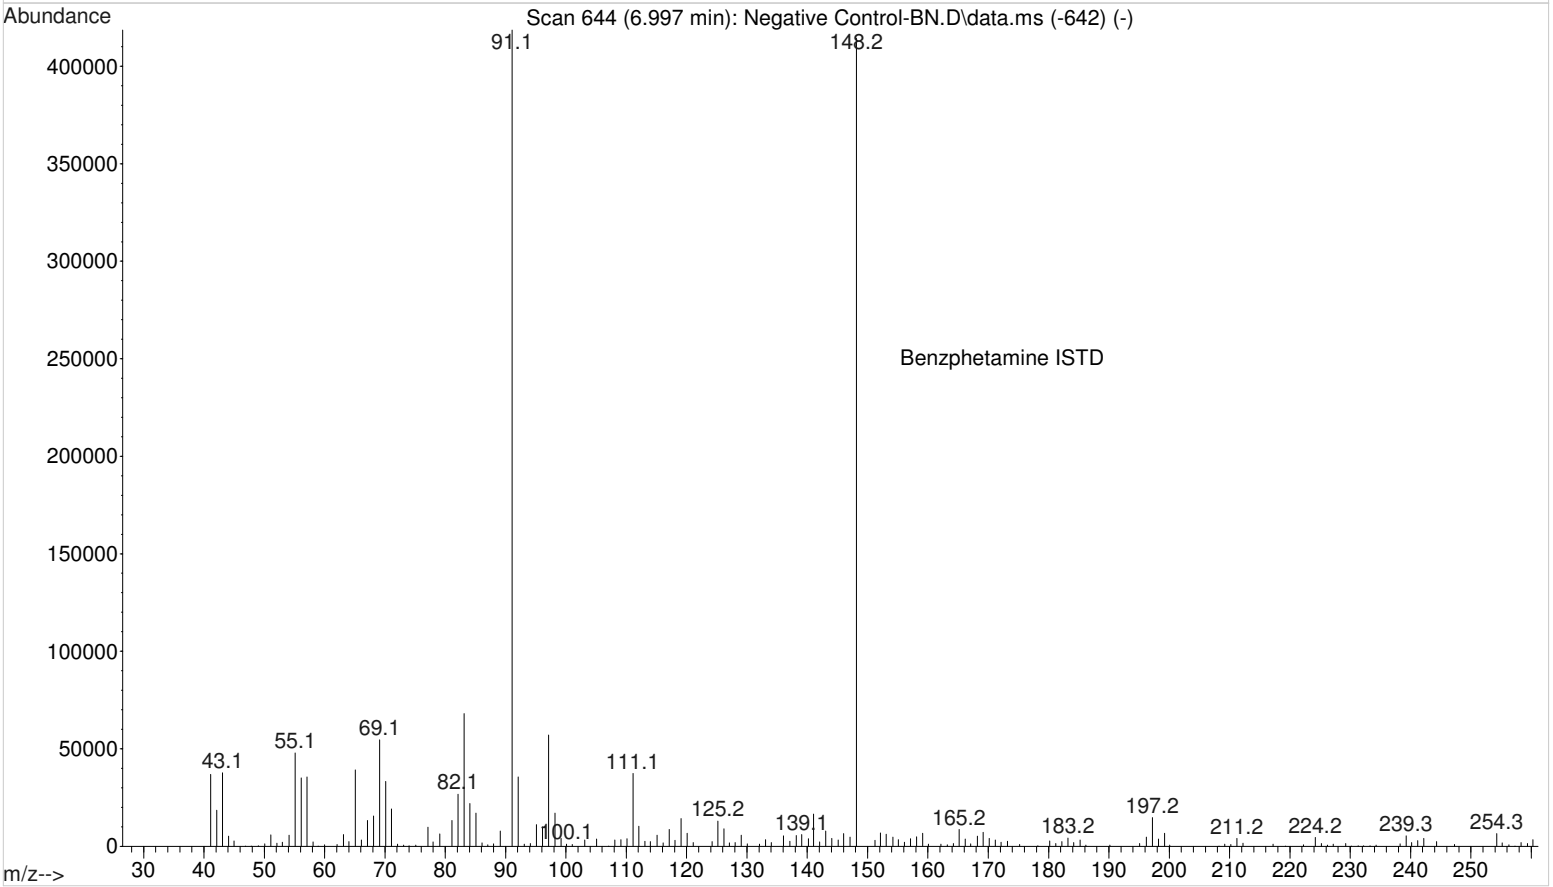

File :I:\Instrument Data\Pocatello\Major Mass Spec\TM\2017\0113201
... 7\Negative Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 13 Jan 2017 16:04 using AcqMethod BNSB120510.M
Sample Name: Negative Control - Utak Lot B1013
Misc Info : Analytical Method 8

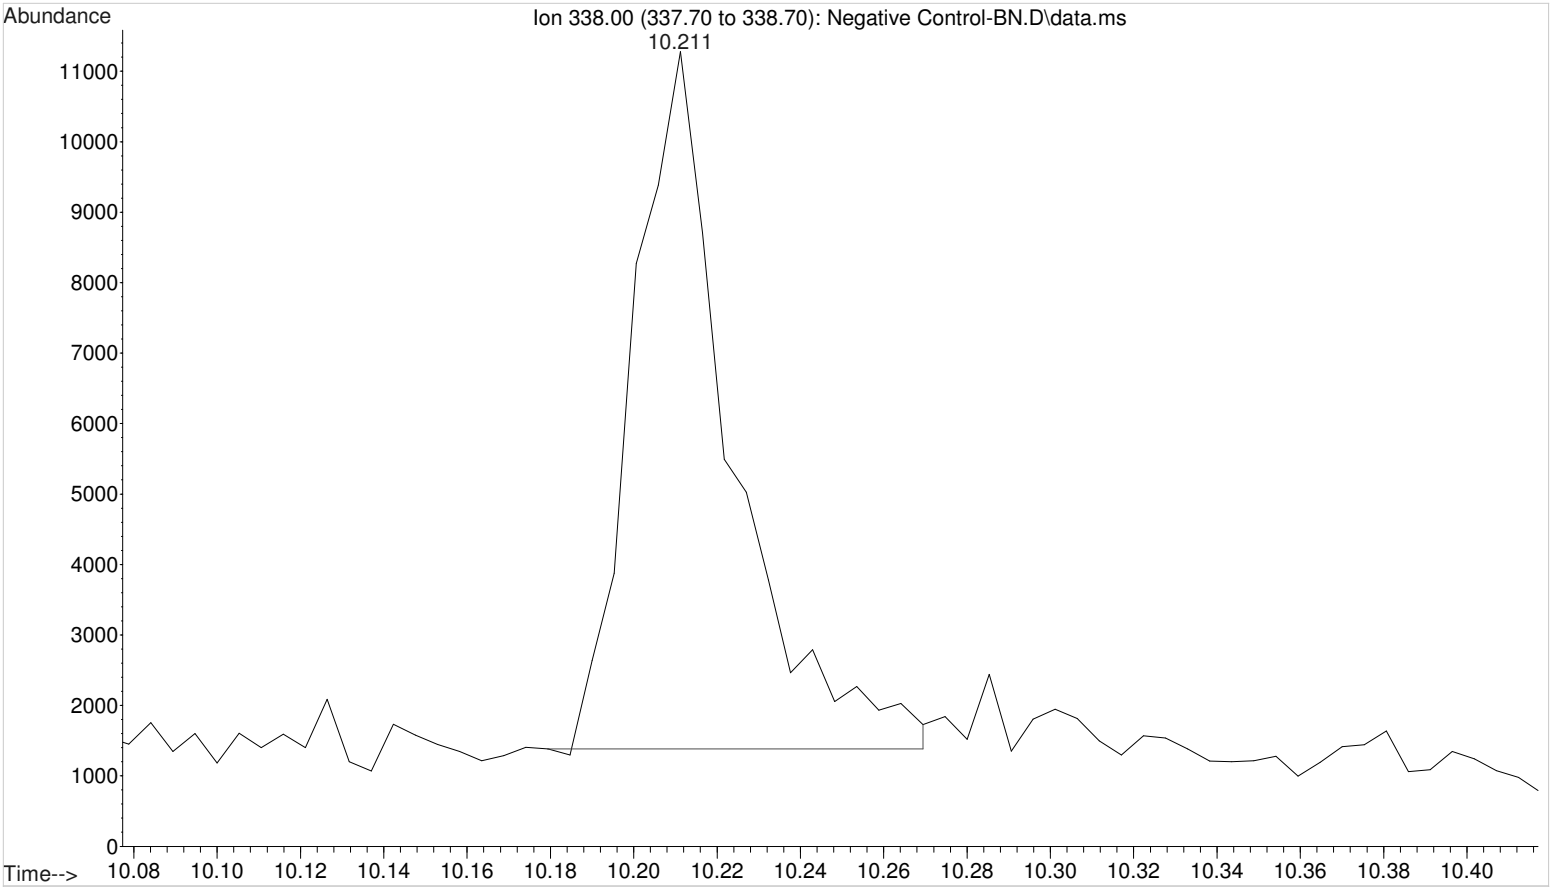

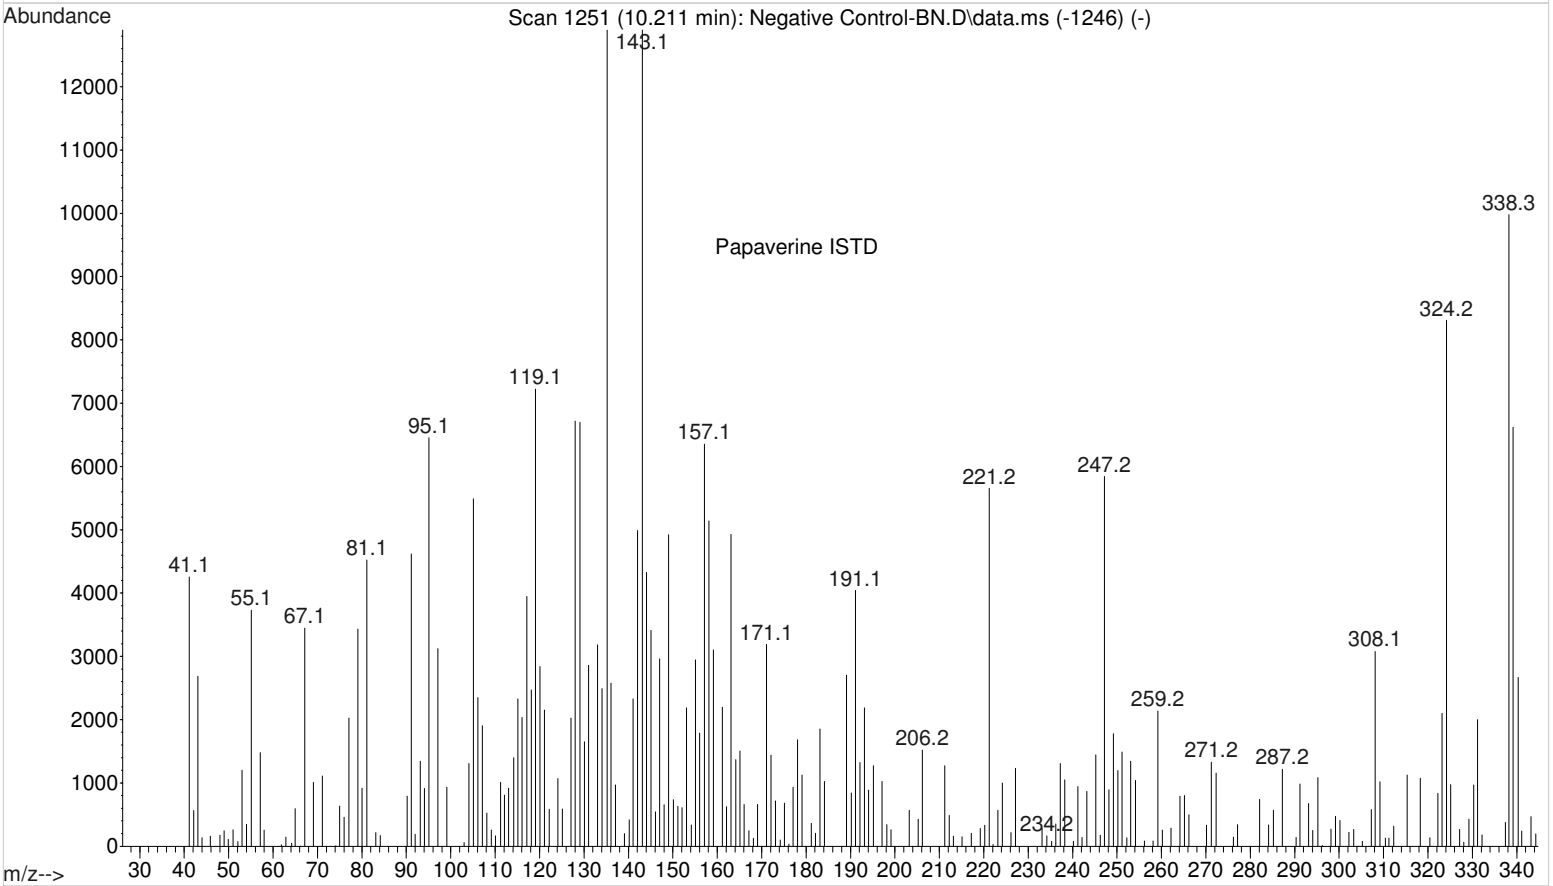

File :I:\Instrument Data\Pocatello\Major Mass Spec\TM\2017\0113201
... 7\Spiked Positive Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 13 Jan 2017 16:27 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

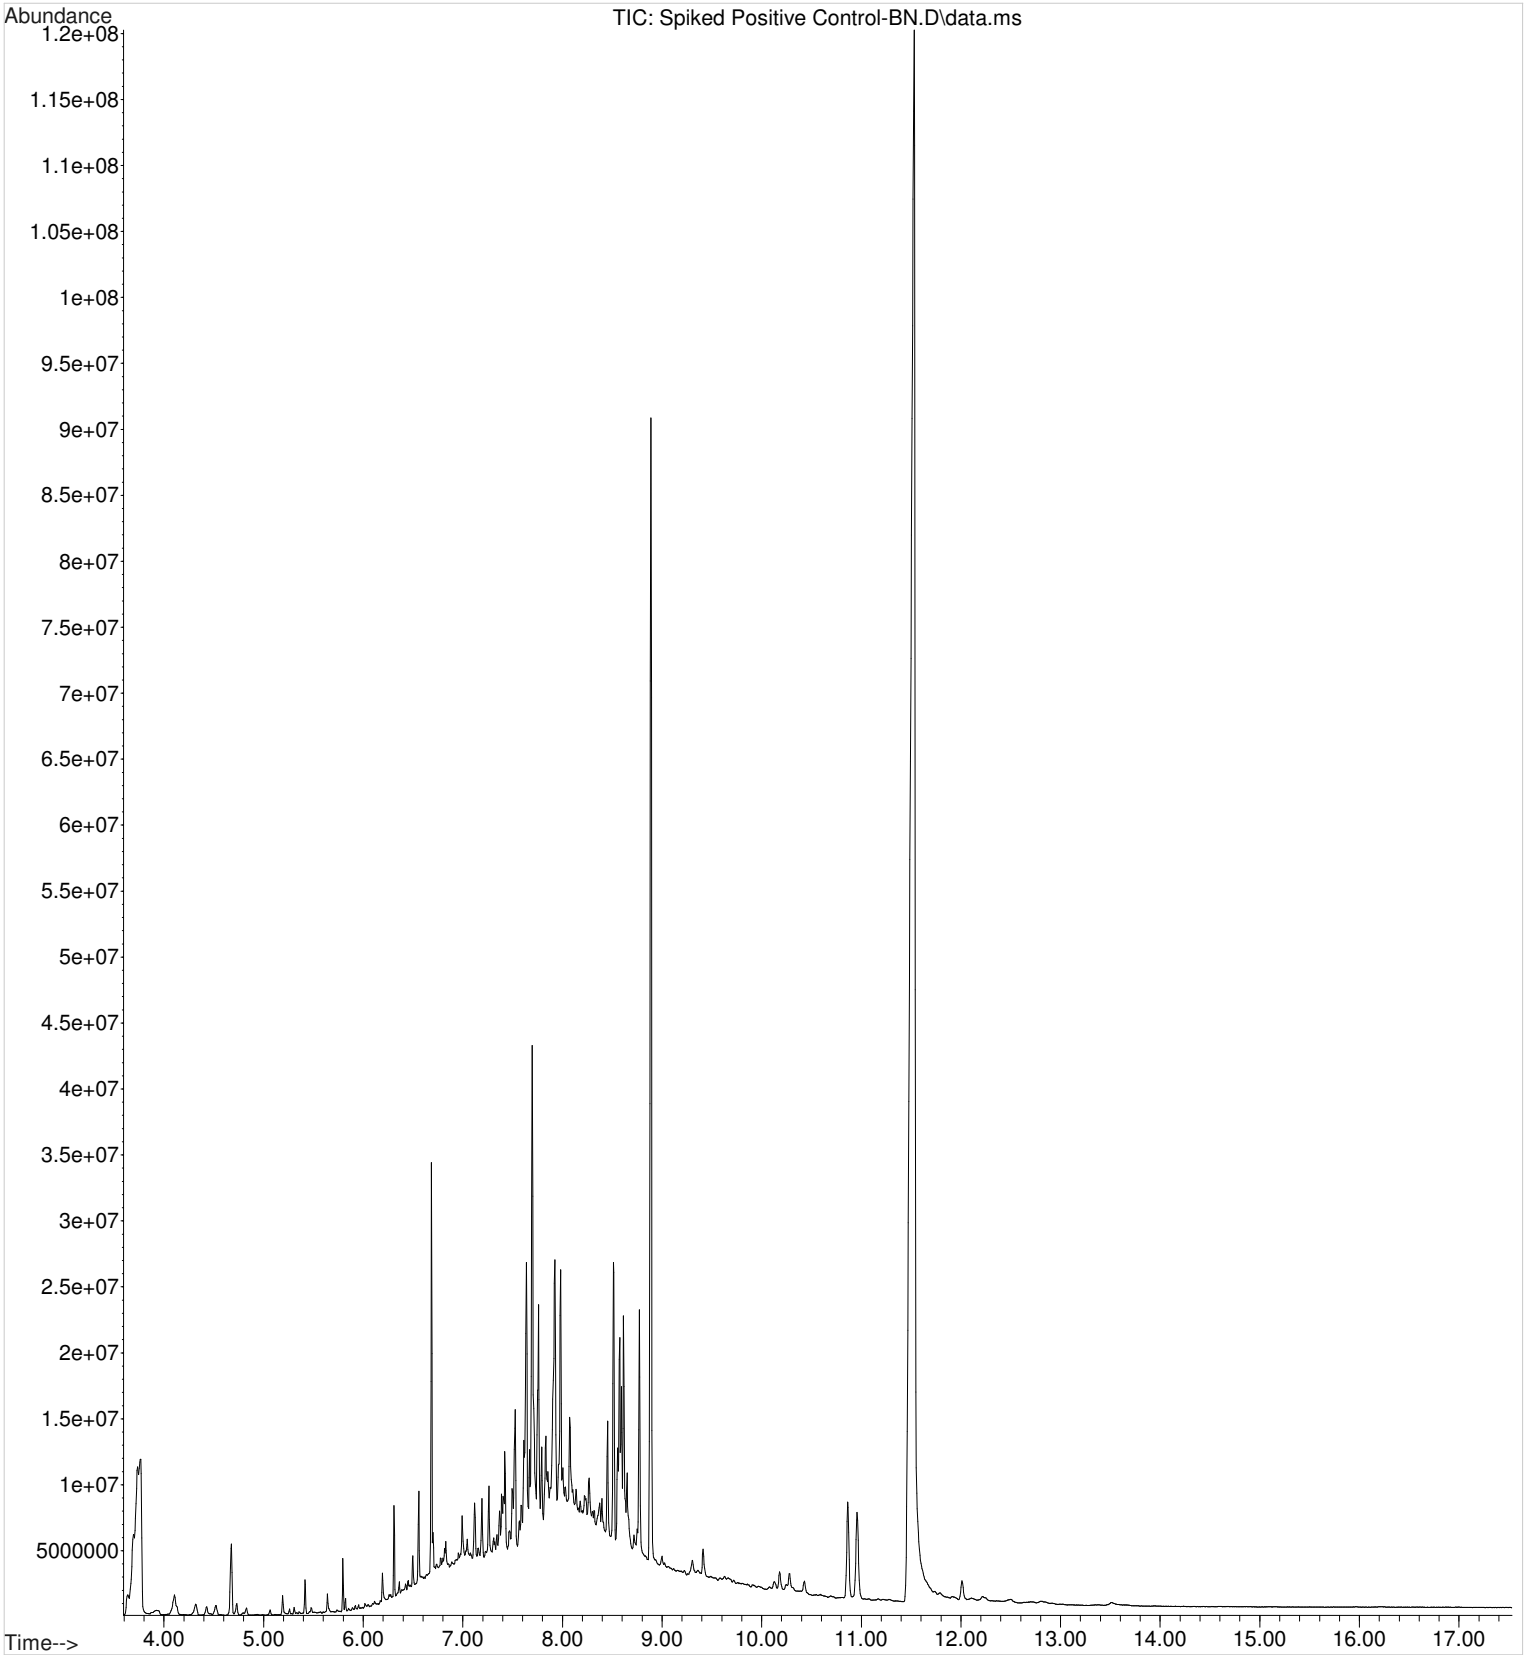

File :I:\Instrument Data\Pocatello\Major Mass Spec\TM\2017\0113201
... 7\Spiked Positive Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 13 Jan 2017 16:27 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

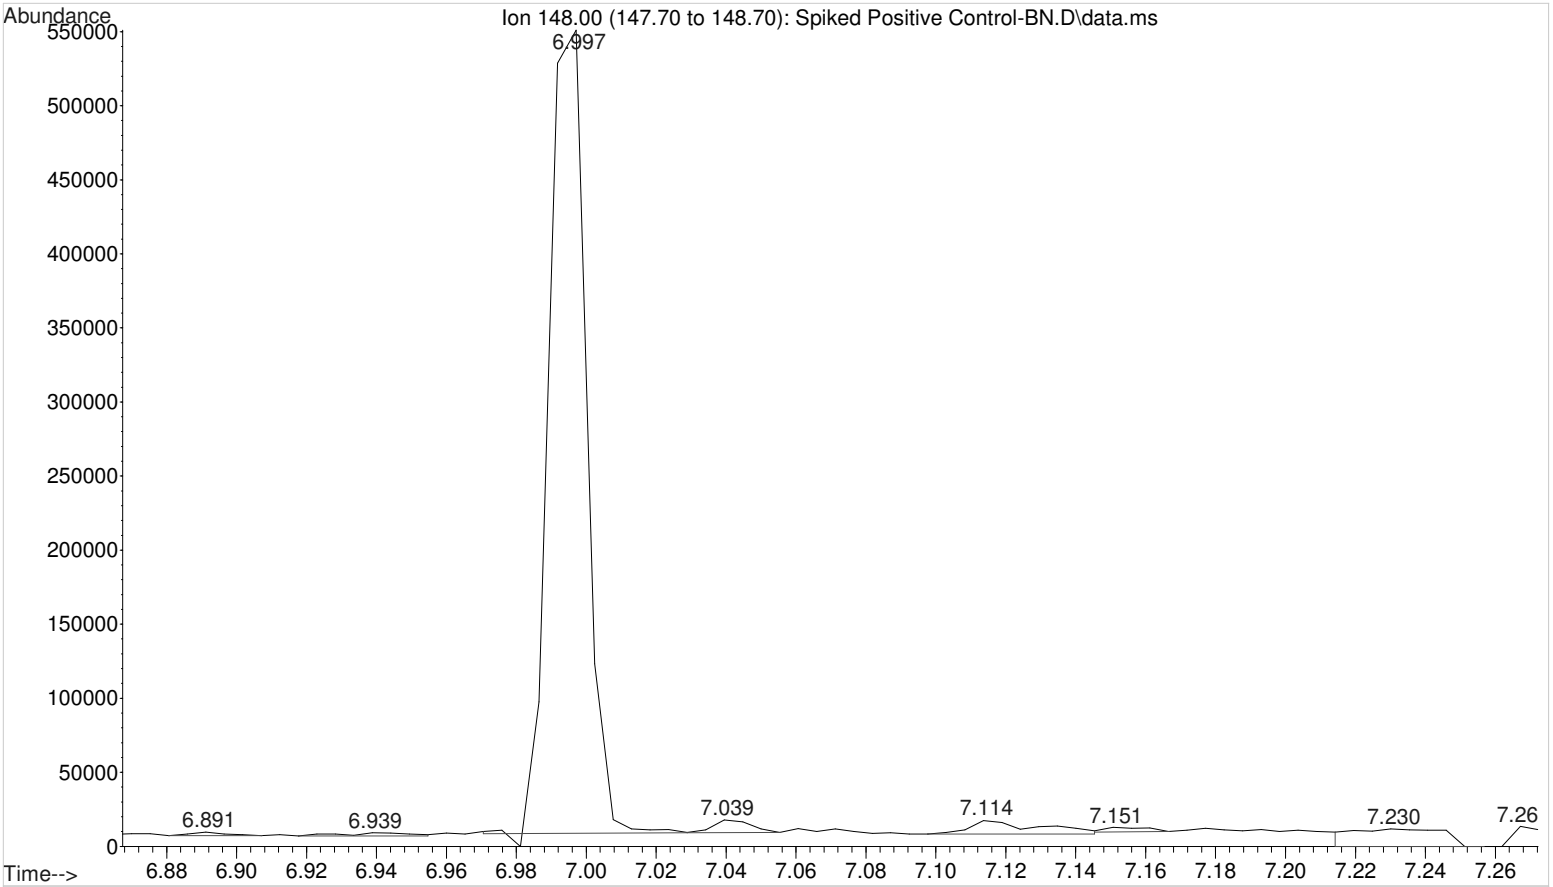

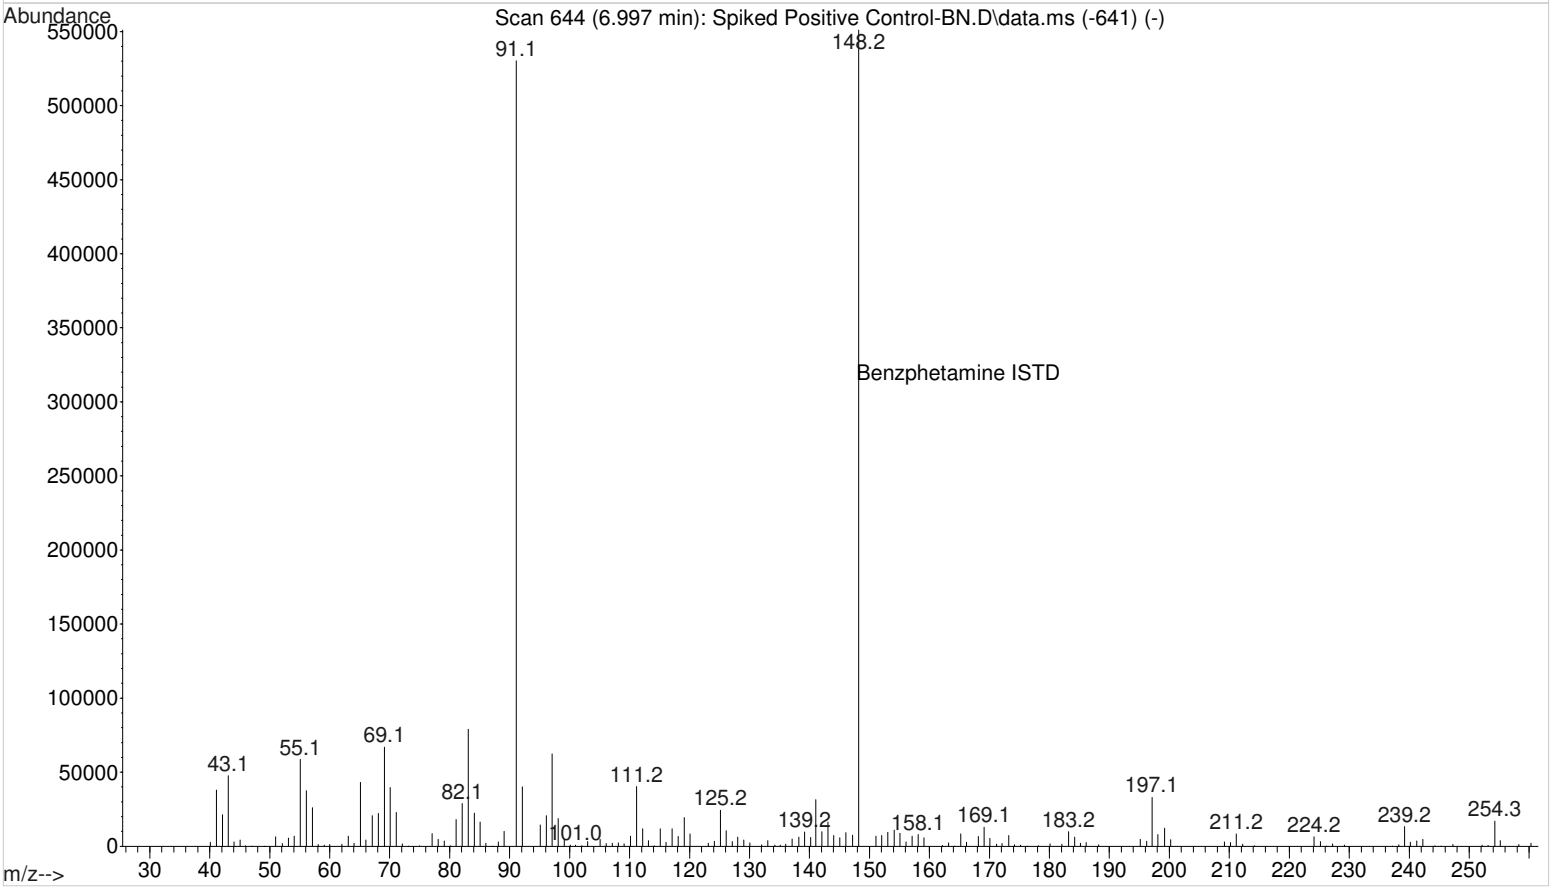

File :I:\Instrument Data\Pocatello\Major Mass Spec\TM\2017\0113201
... 7\Spiked Positive Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 13 Jan 2017 16:27 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

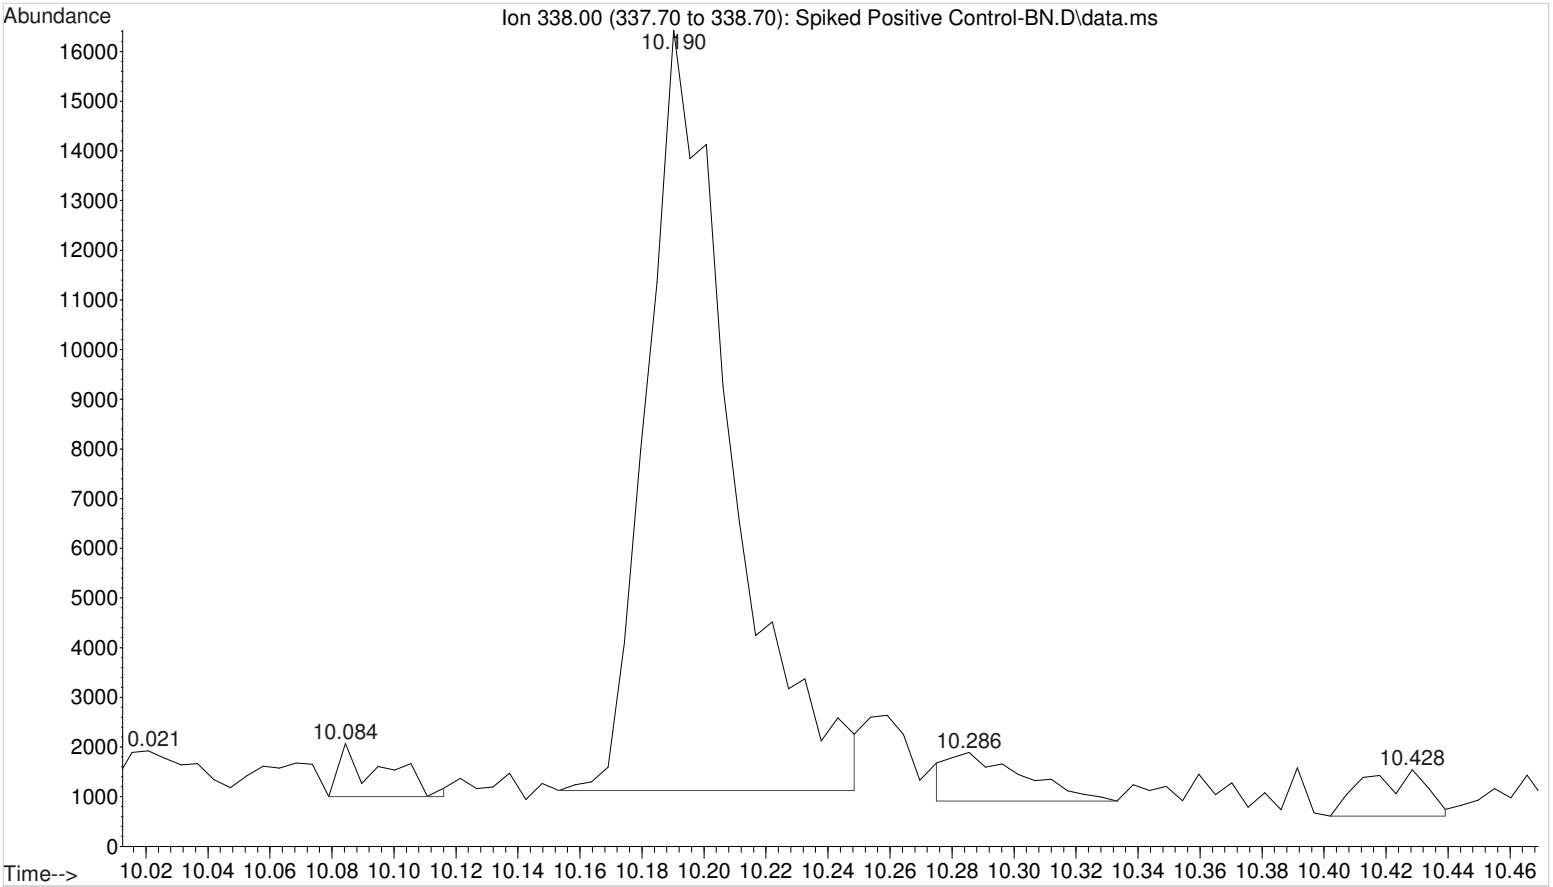

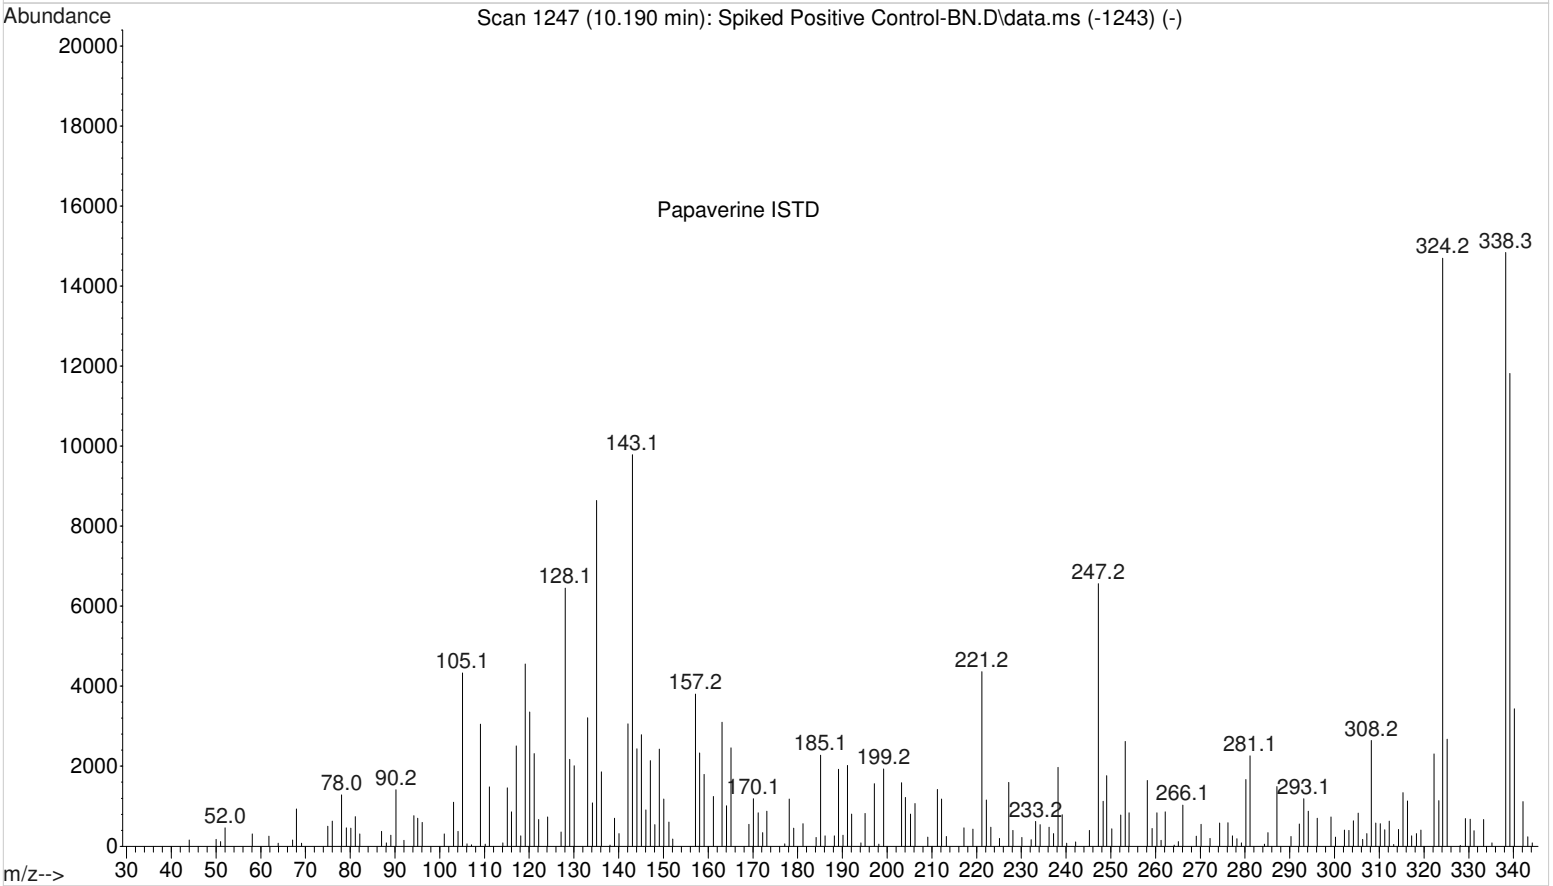

File :I:\Instrument Data\Pocatello\Major Mass Spec\TM\2017\0113201
... 7\Spiked Positive Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 13 Jan 2017 16:27 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

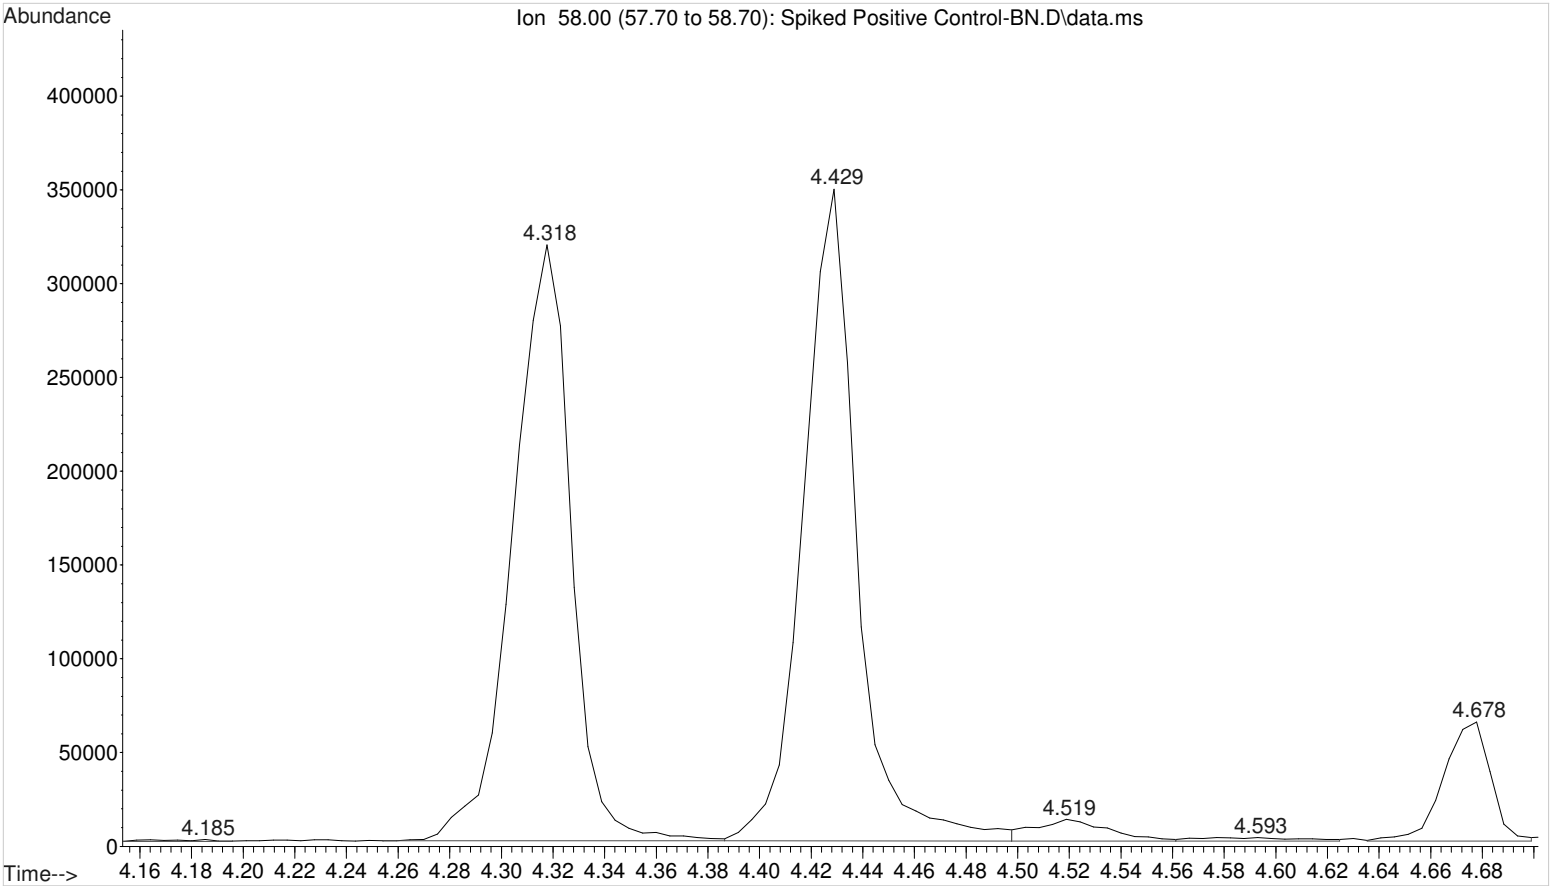

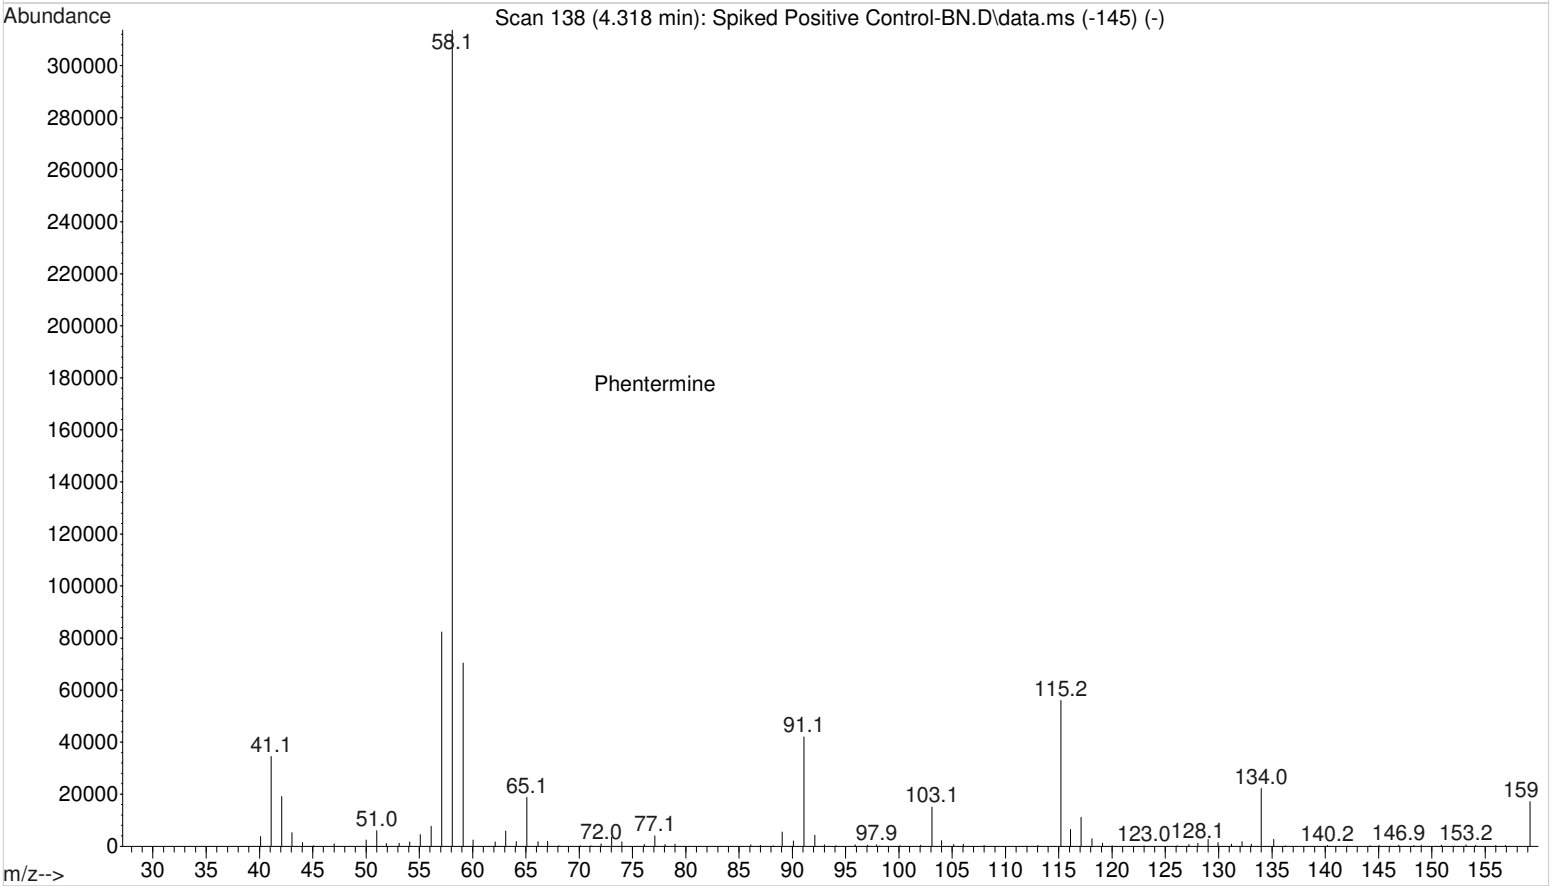

File :I:\Instrument Data\Pocatello\Major Mass Spec\TM\2017\0113201
... 7\Spiked Positive Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 13 Jan 2017 16:27 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

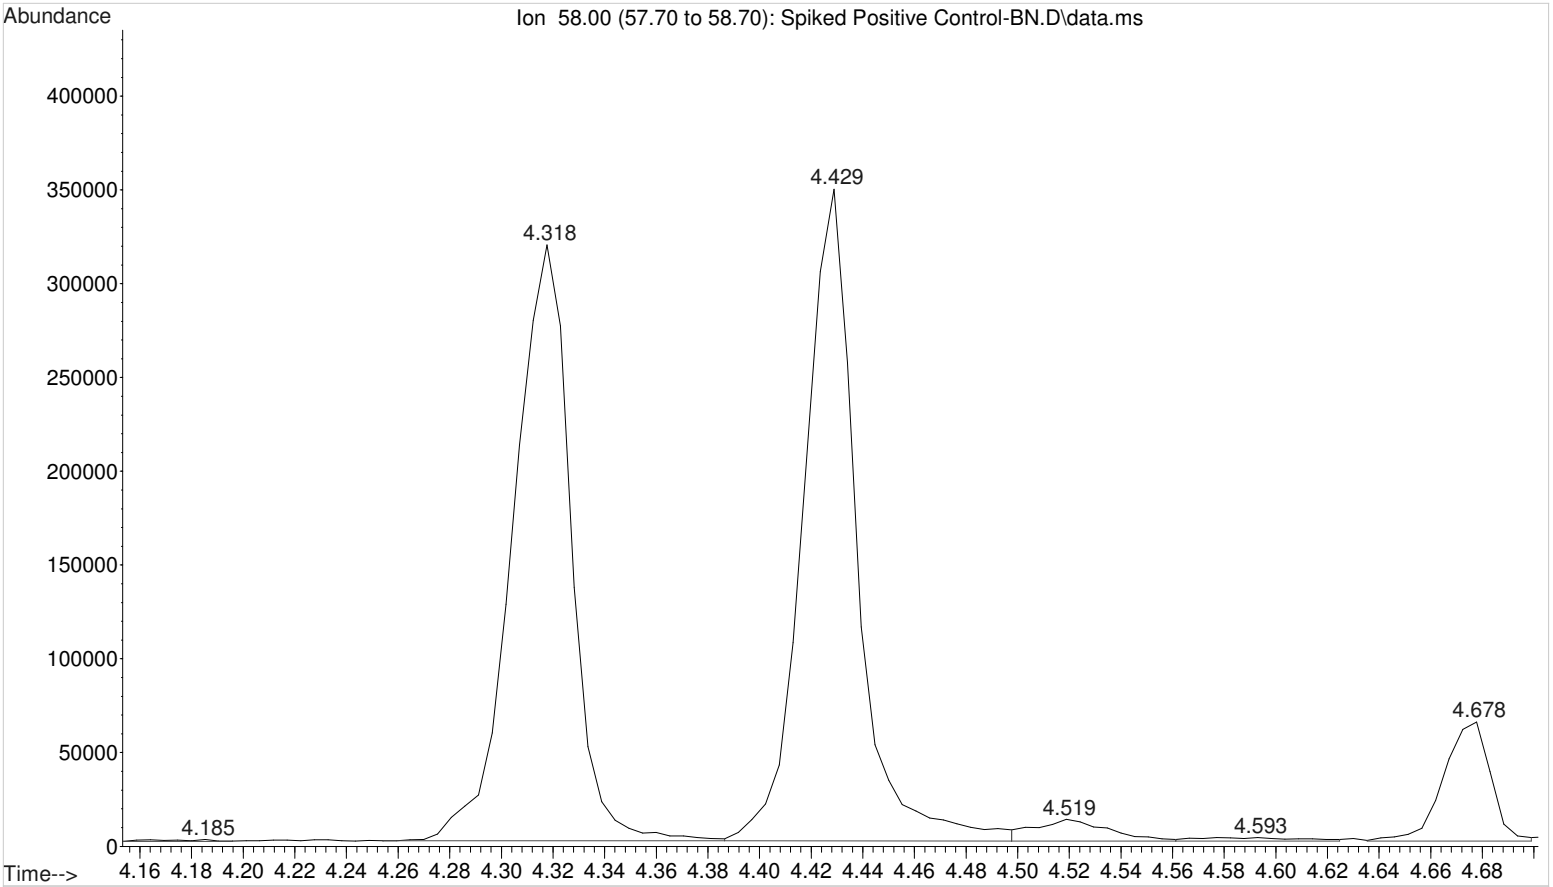

File :I:\Instrument Data\Pocatello\Major Mass Spec\TM\2017\0113201
... 7\Spiked Positive Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 13 Jan 2017 16:27 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

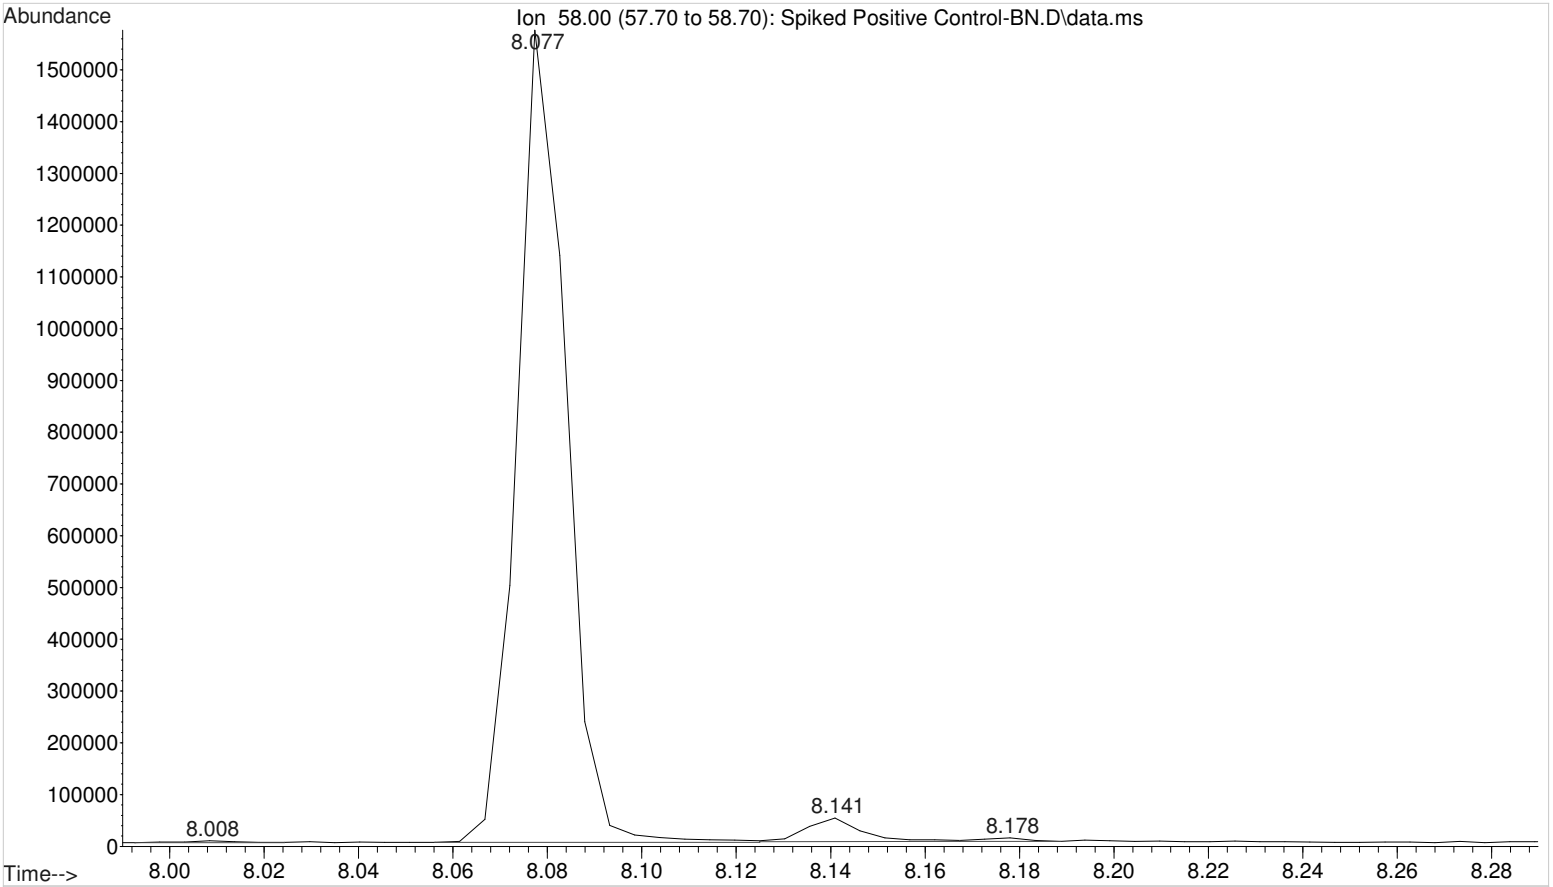

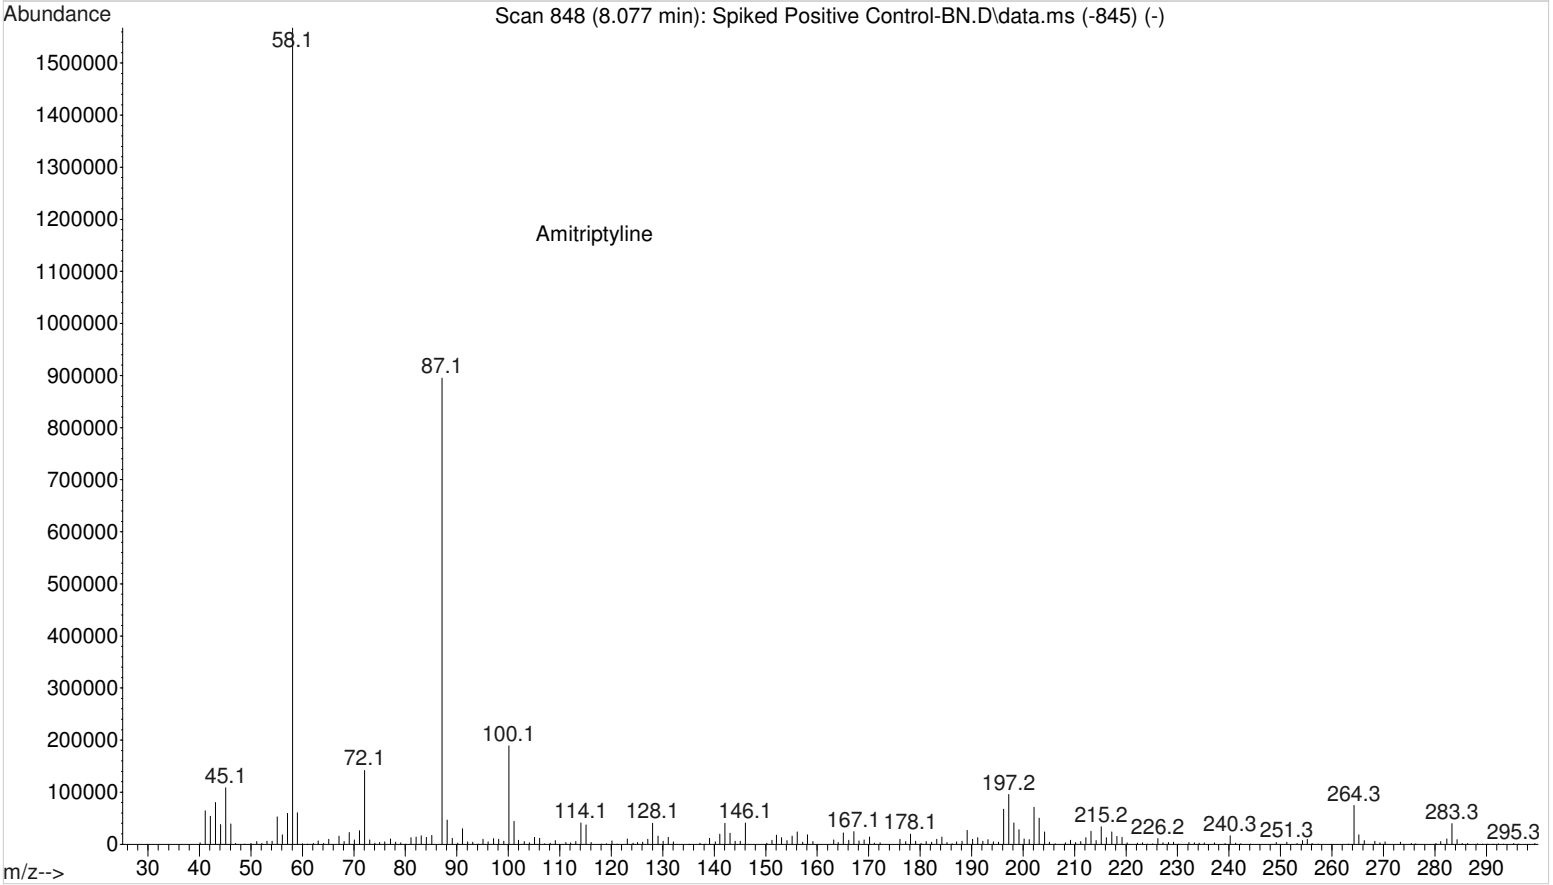

File :I:\Instrument Data\Pocatello\Major Mass Spec\TM\2017\0113201
... 7\Spiked Positive Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 13 Jan 2017 16:27 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

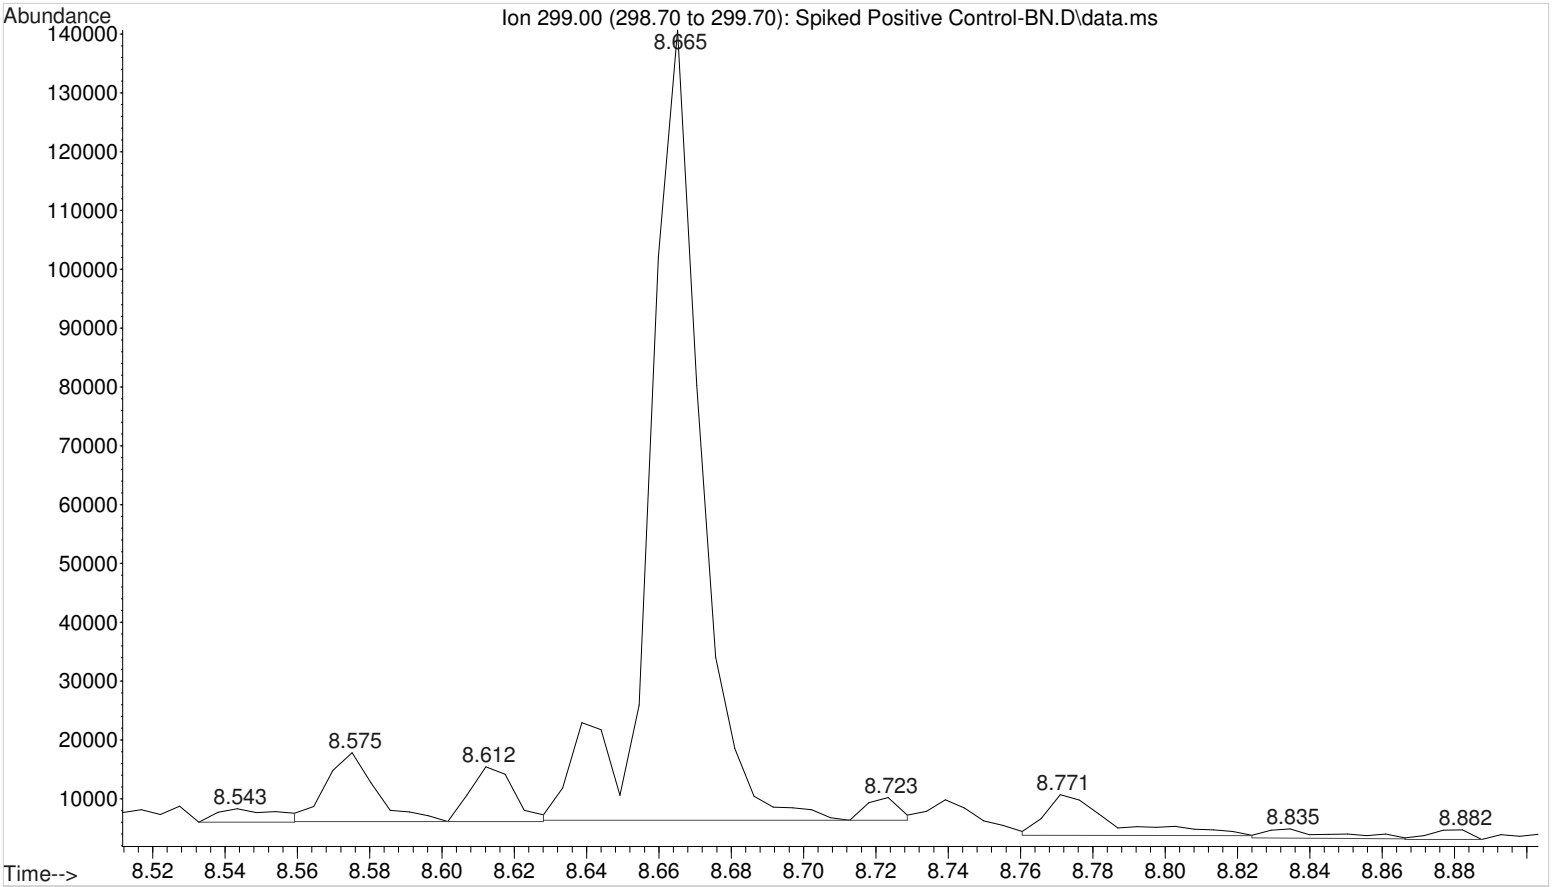

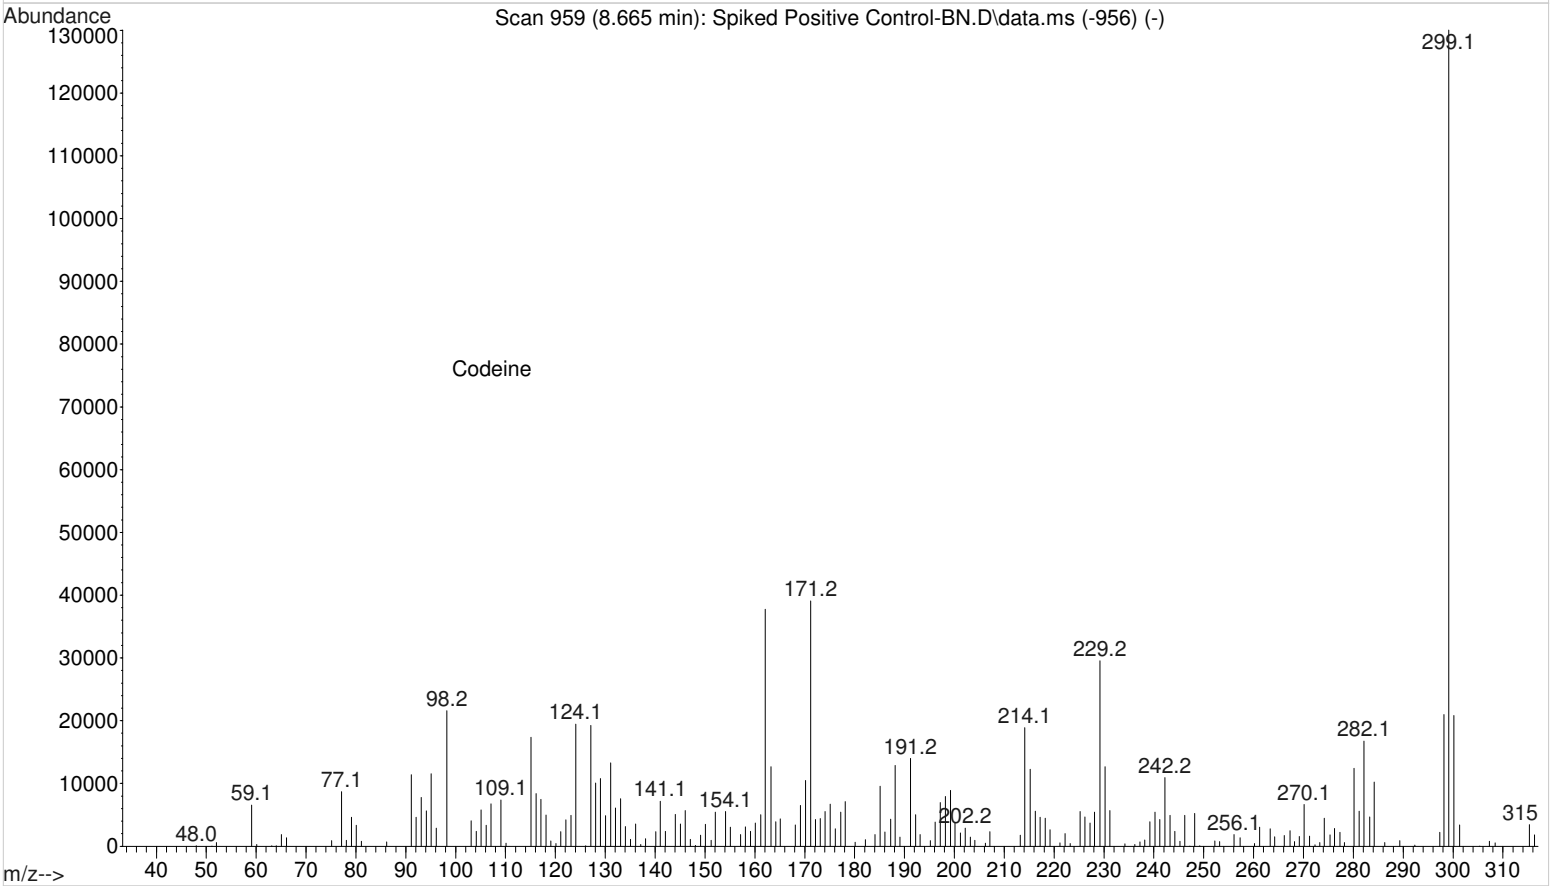

File :I:\Instrument Data\Pocatello\Major Mass Spec\TM\2017\0113201
... 7\Spiked Positive Control-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 13 Jan 2017 16:27 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

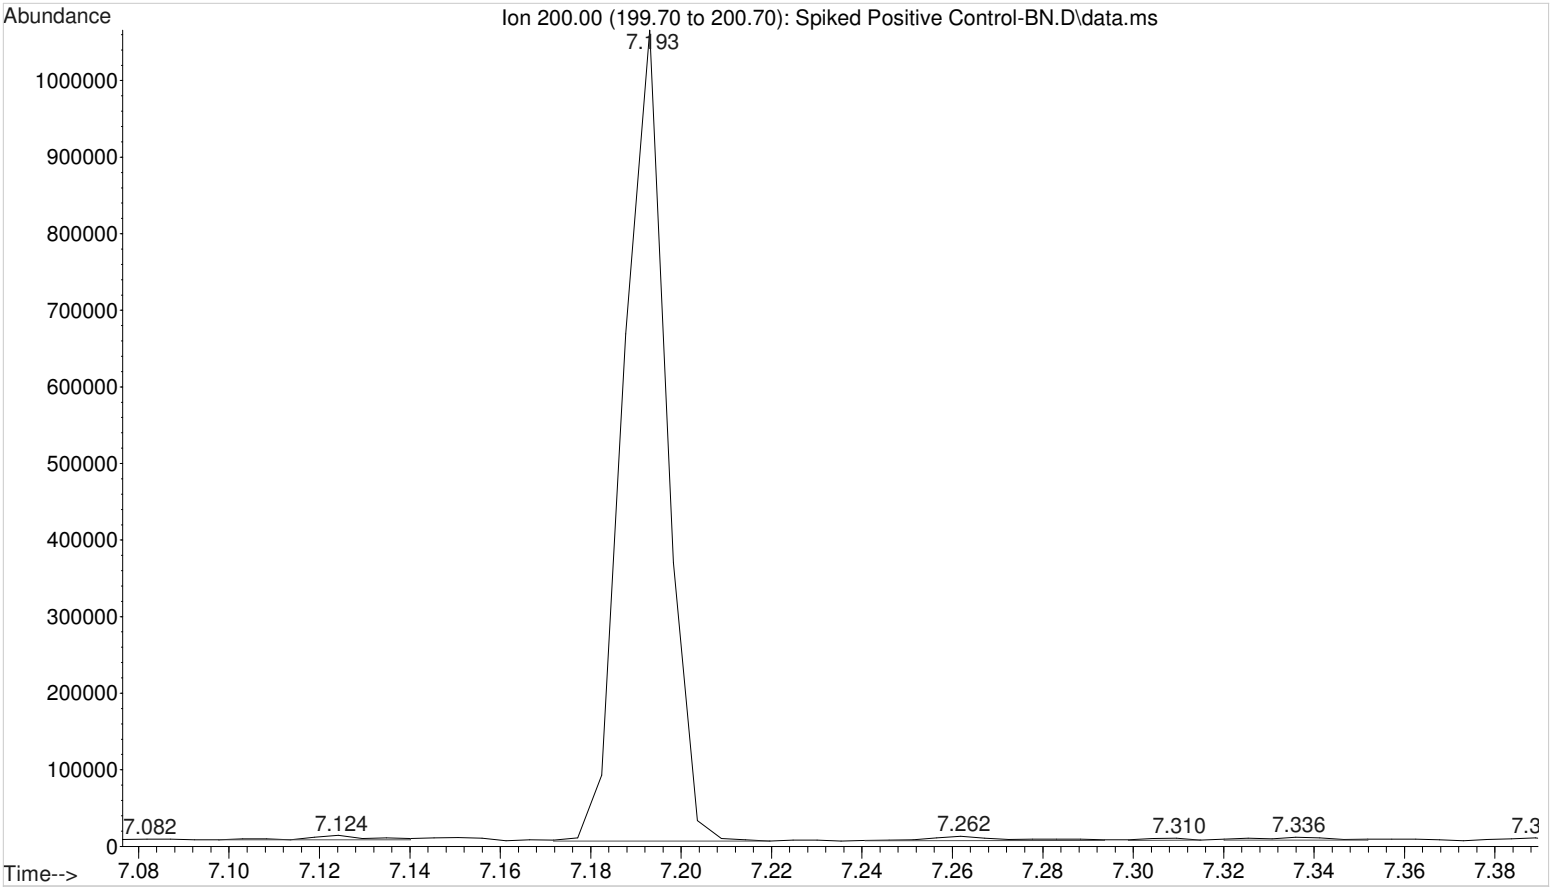

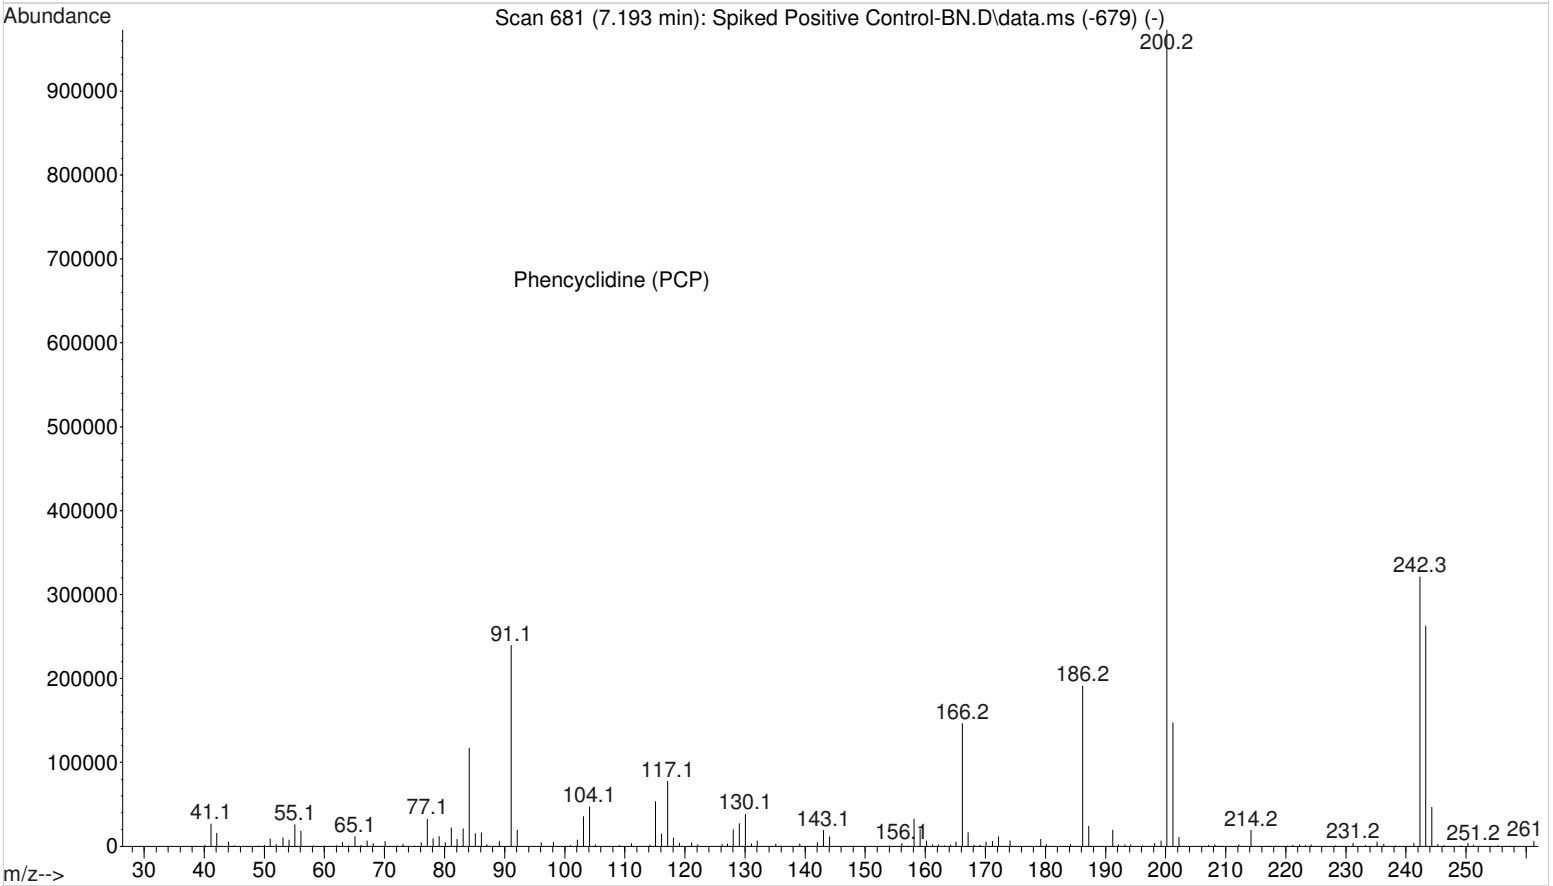

File :I:\Instrument Data\Pocatello\Major Mass Spec\TM\2017\0113201
... 7\Negative Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 13 Jan 2017 17:46 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Negative Control - Utak Lot B1013
Misc Info : Analytical Method 8

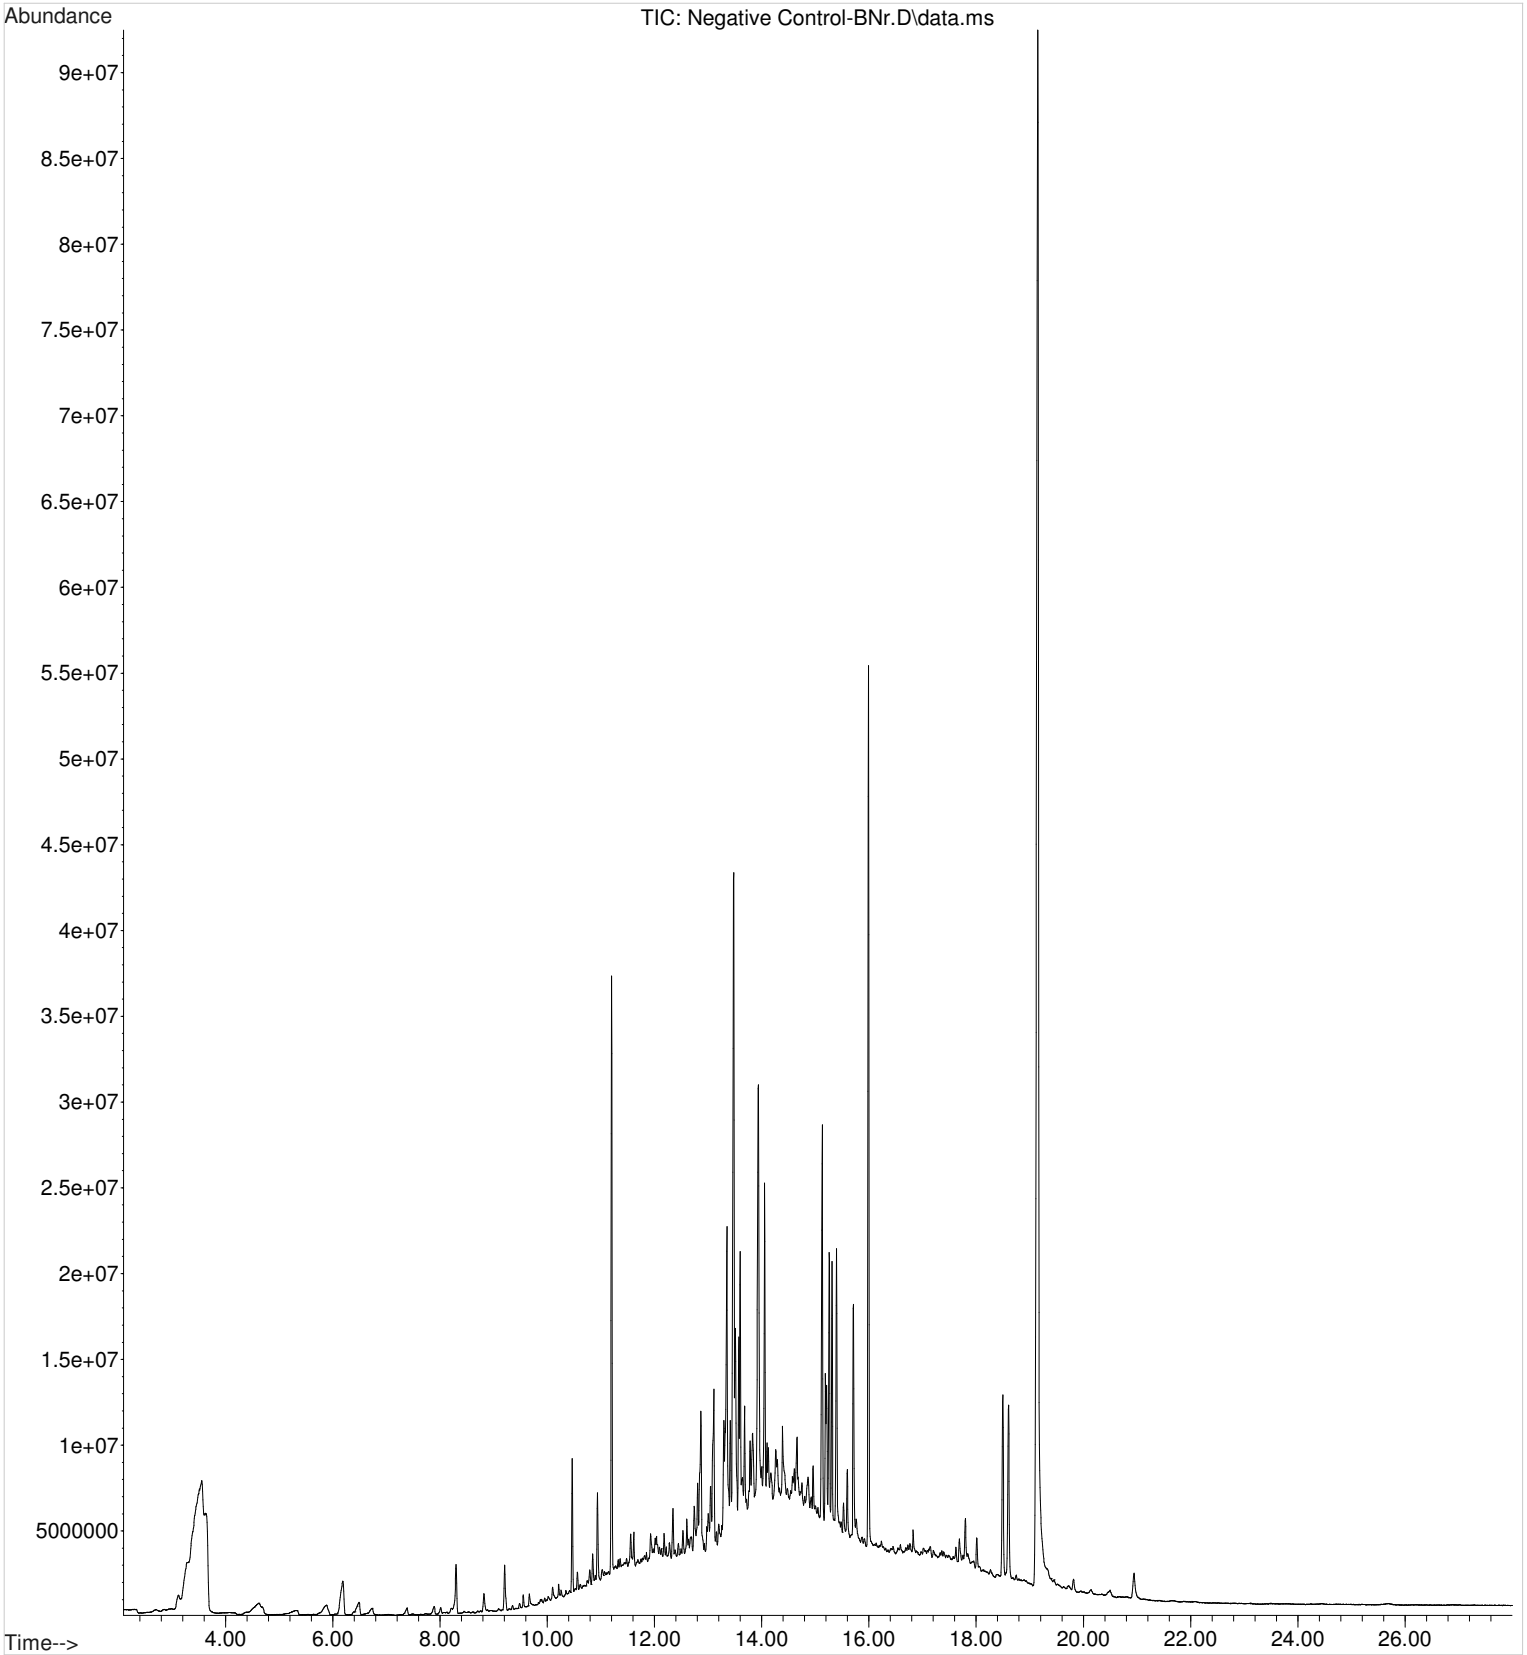

File :I:\Instrument Data\Pocatello\Major Mass Spec\TM\2017\0113201
... 7\Negative Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 13 Jan 2017 17:46 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Negative Control - Utak Lot B1013
Misc Info : Analytical Method 8

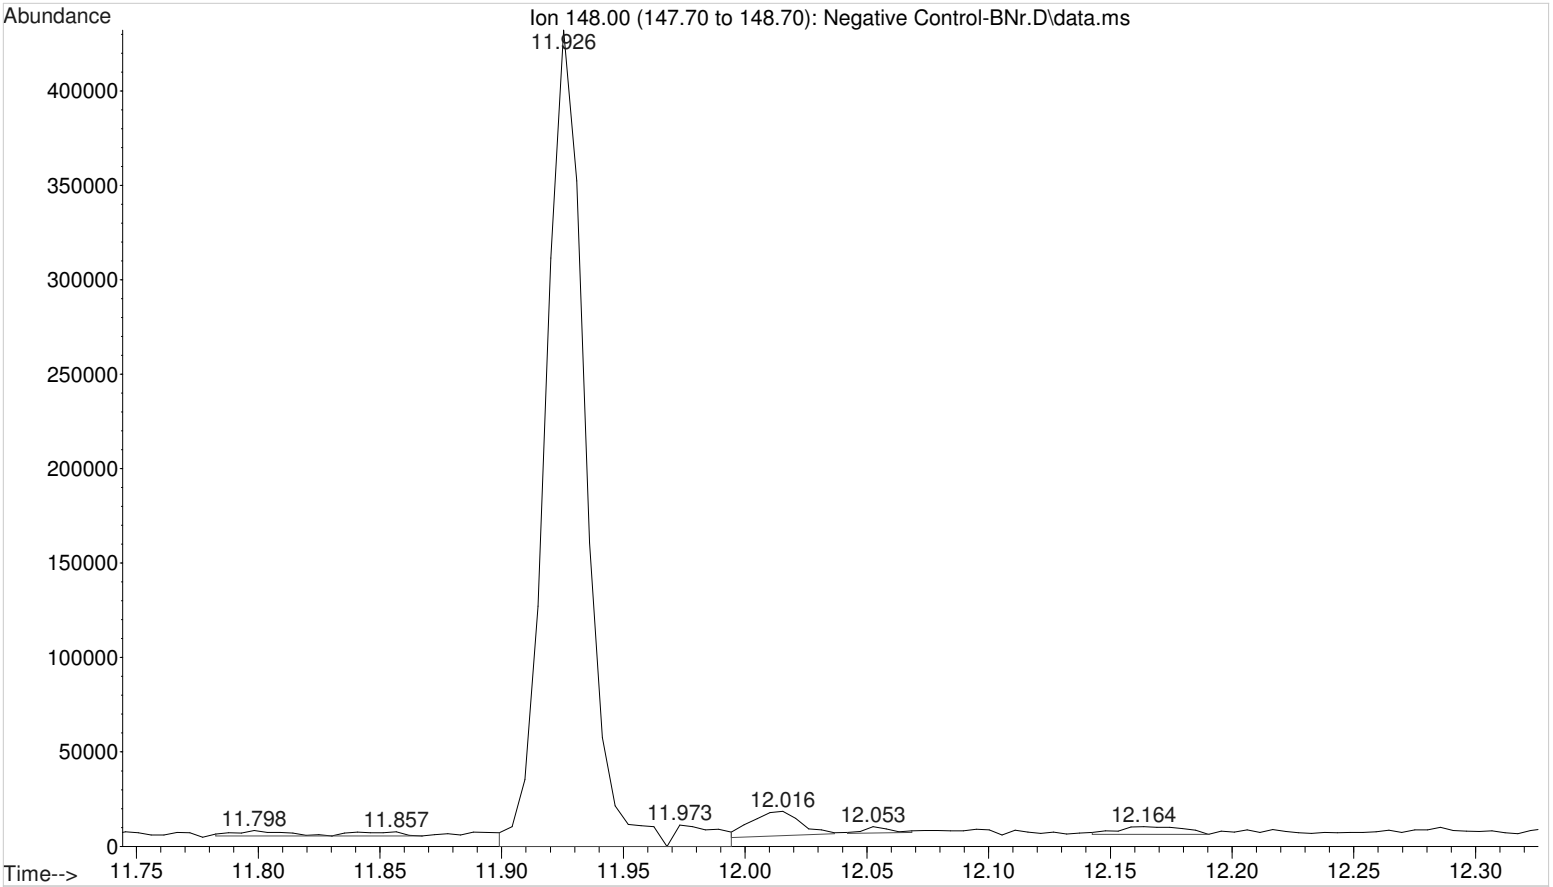

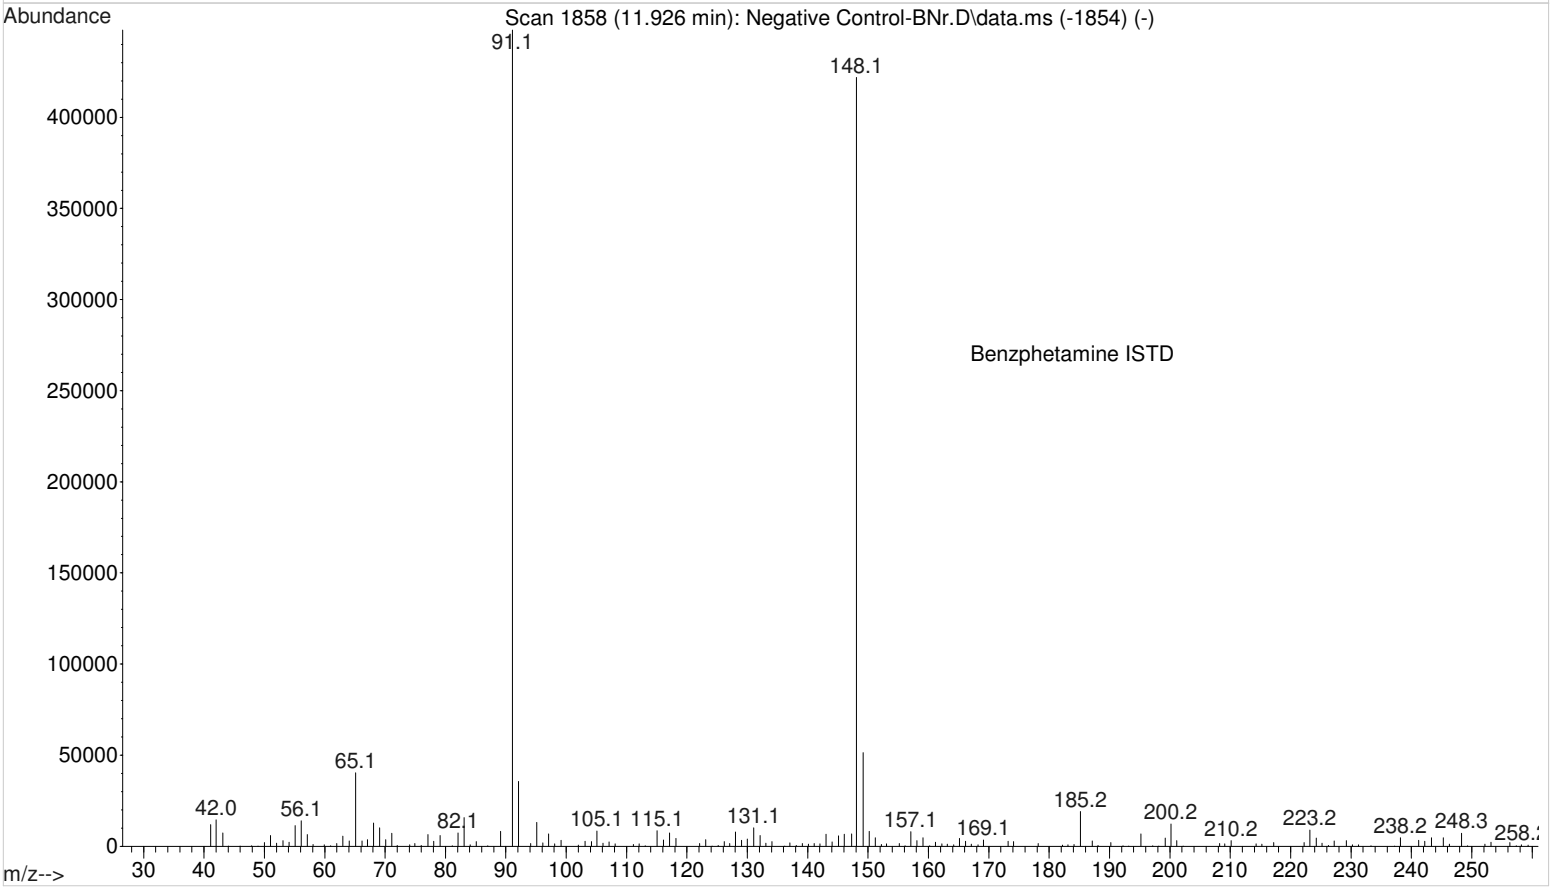

File :I:\Instrument Data\Pocatello\Major Mass Spec\TM\2017\0113201
... 7\Negative Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 13 Jan 2017 17:46 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Negative Control - Utak Lot B1013
Misc Info : Analytical Method 8

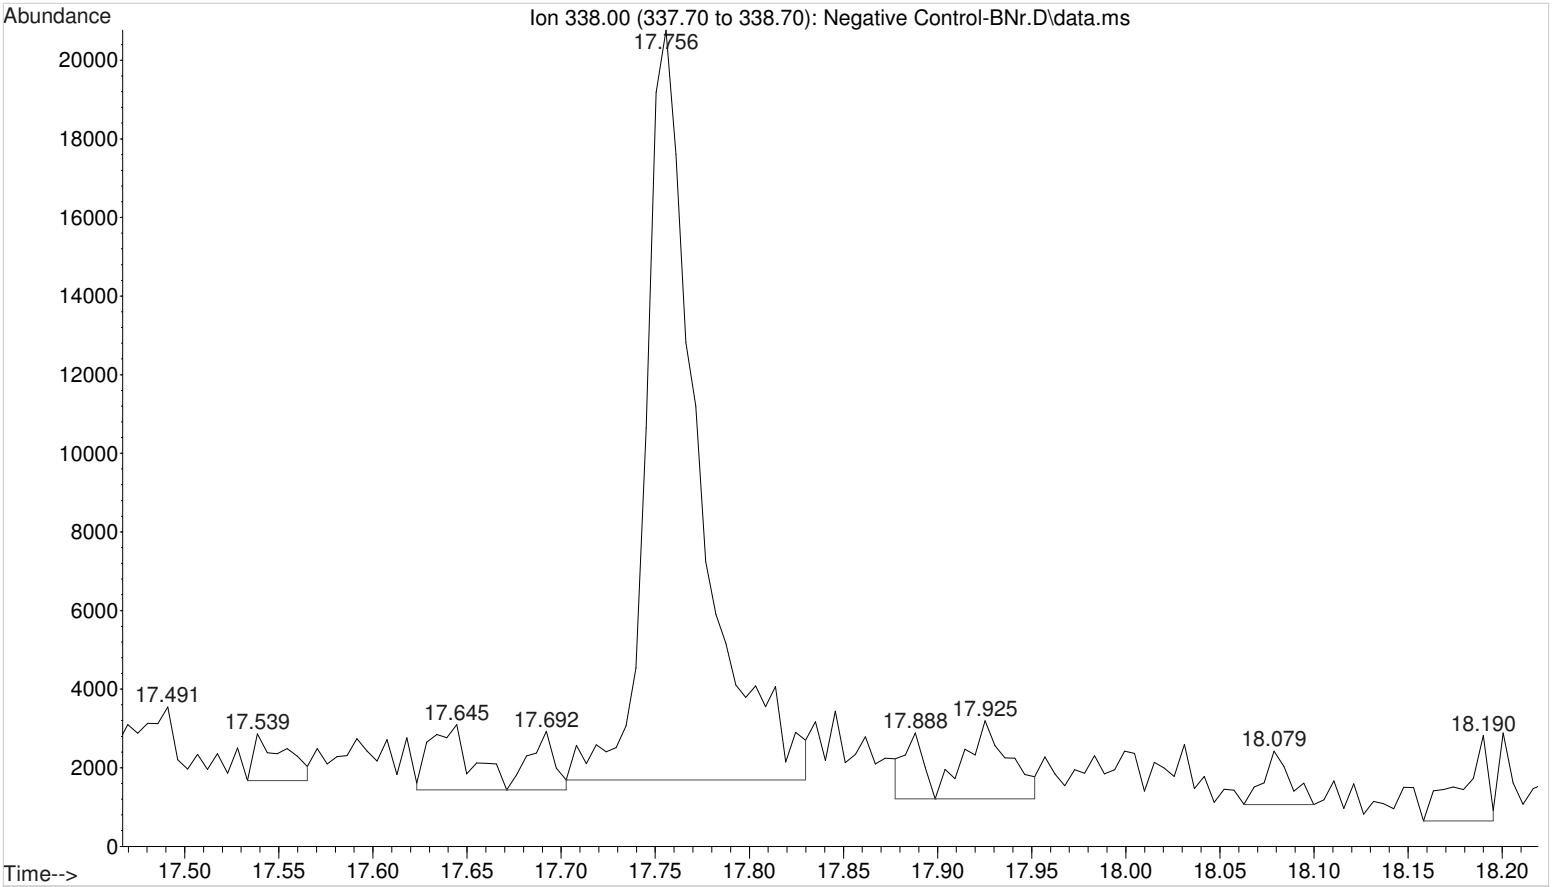

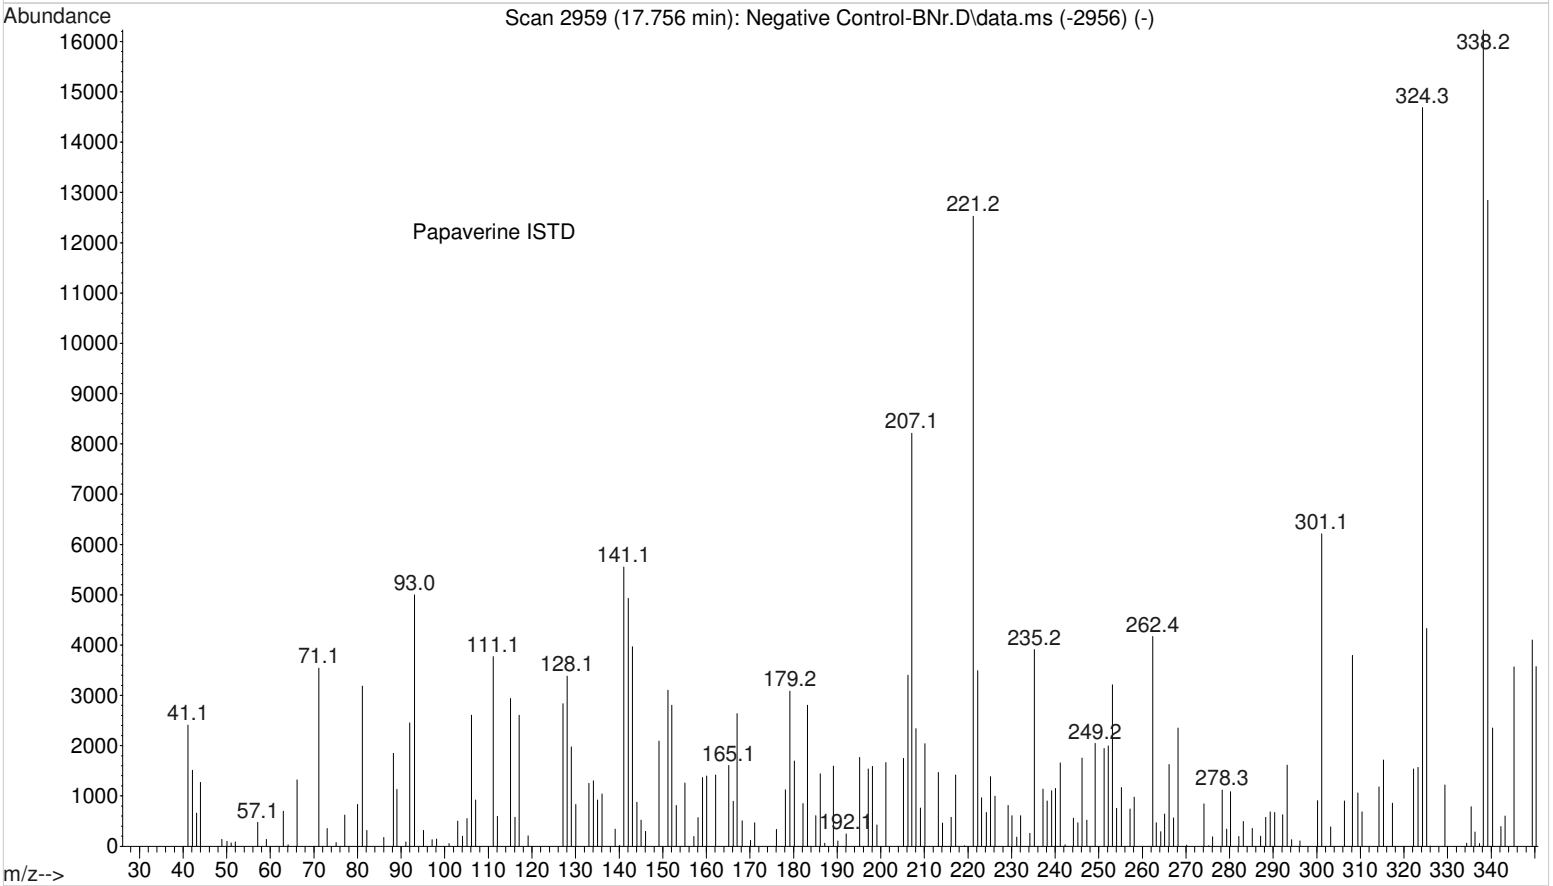

File :I:\Instrument Data\Pocatello\Major Mass Spec\TM\2017\0113201
... 7\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 13 Jan 2017 18:20 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

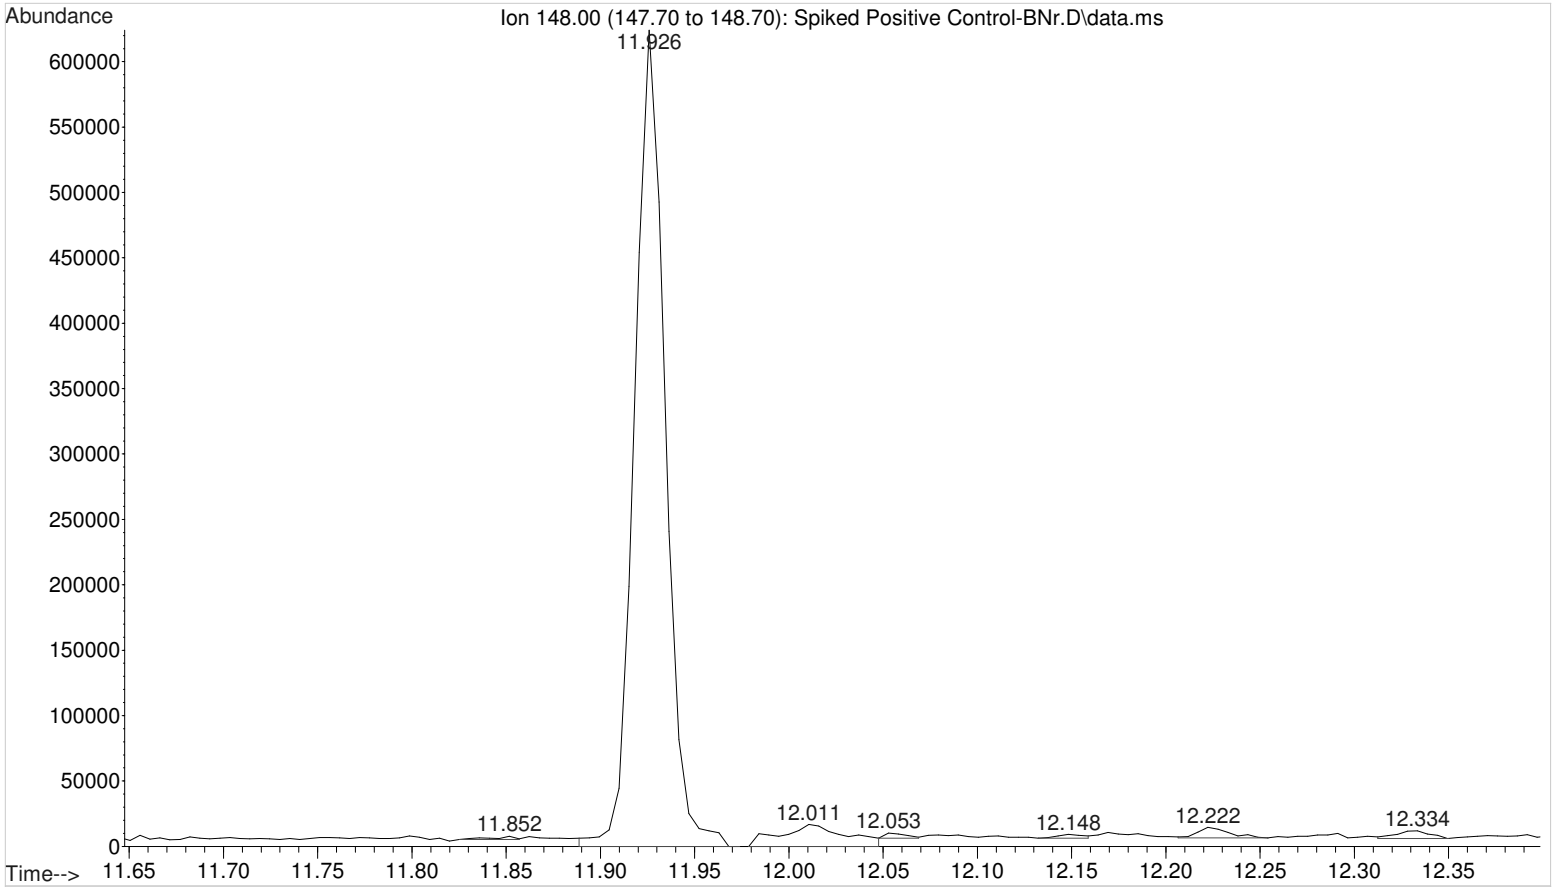

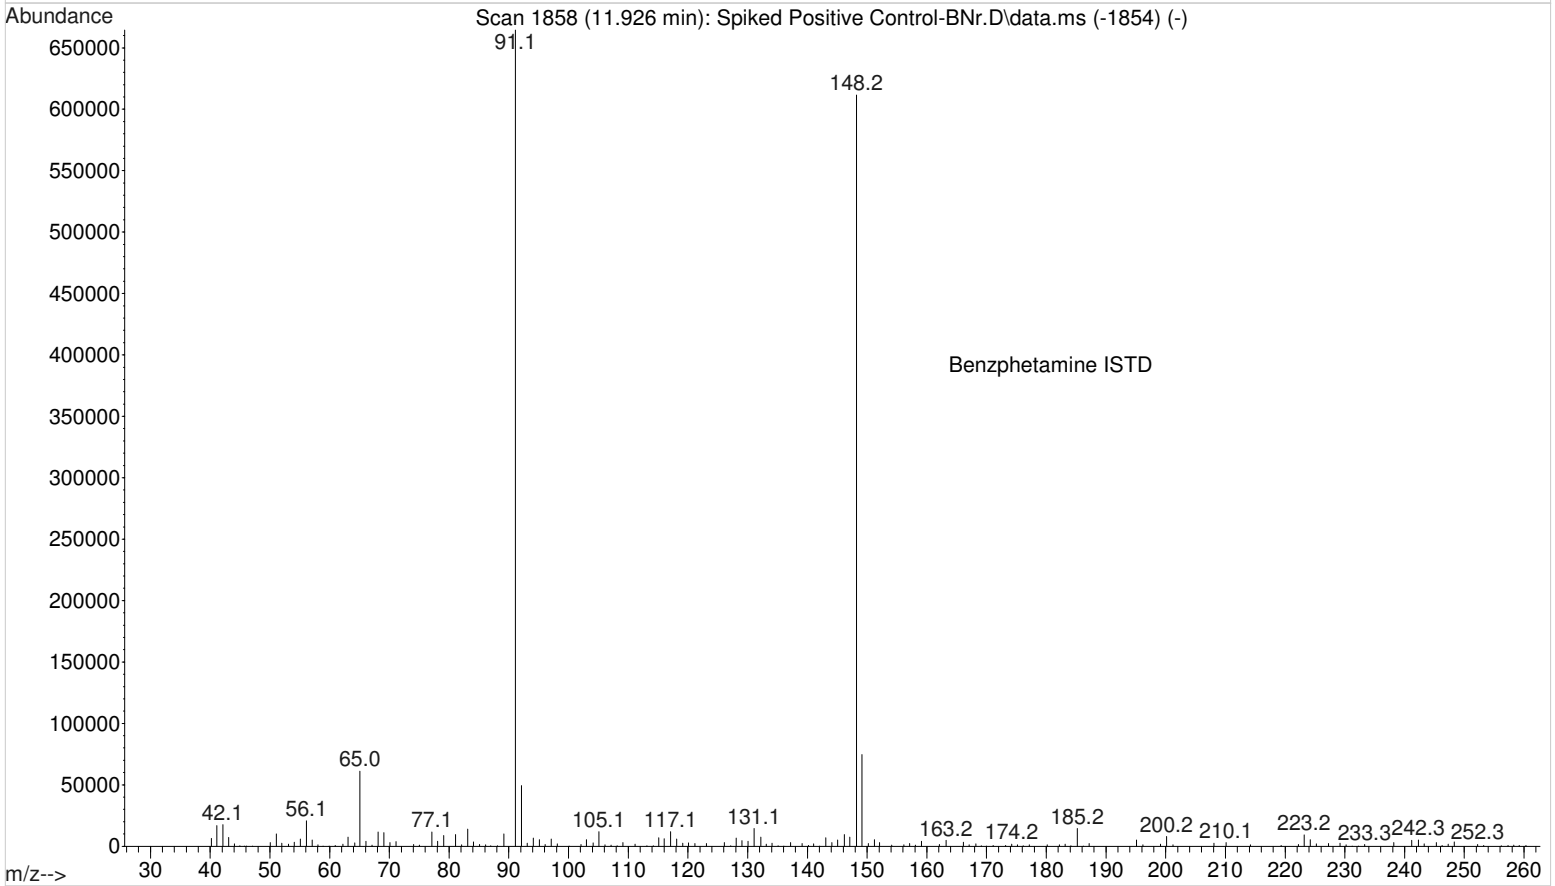

File :I:\Instrument Data\Pocatello\Major Mass Spec\TM\2017\0113201
... 7\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 13 Jan 2017 18:20 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

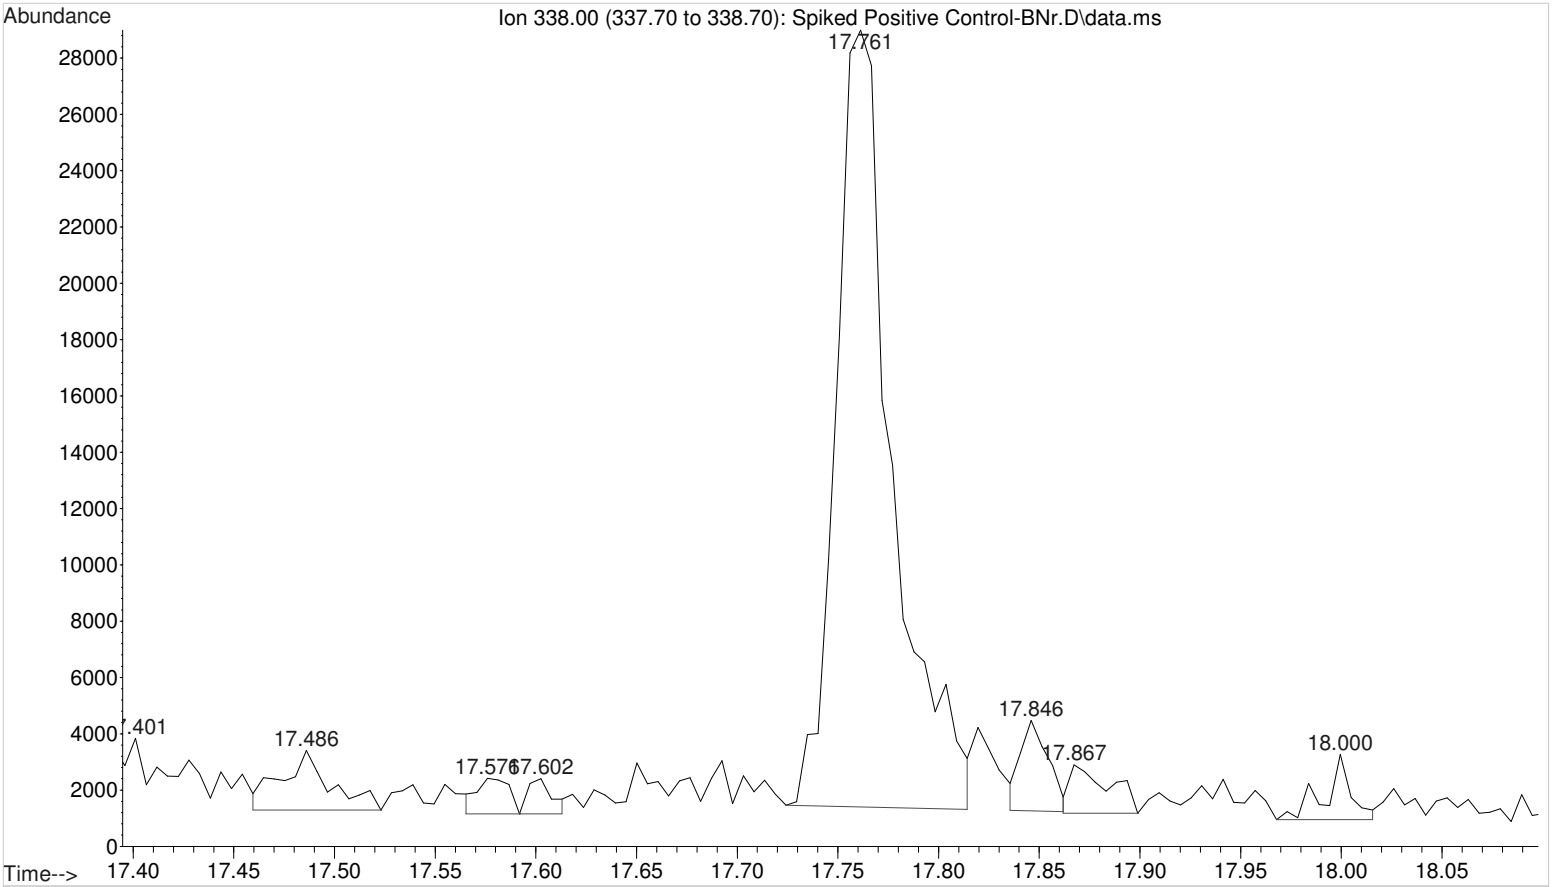

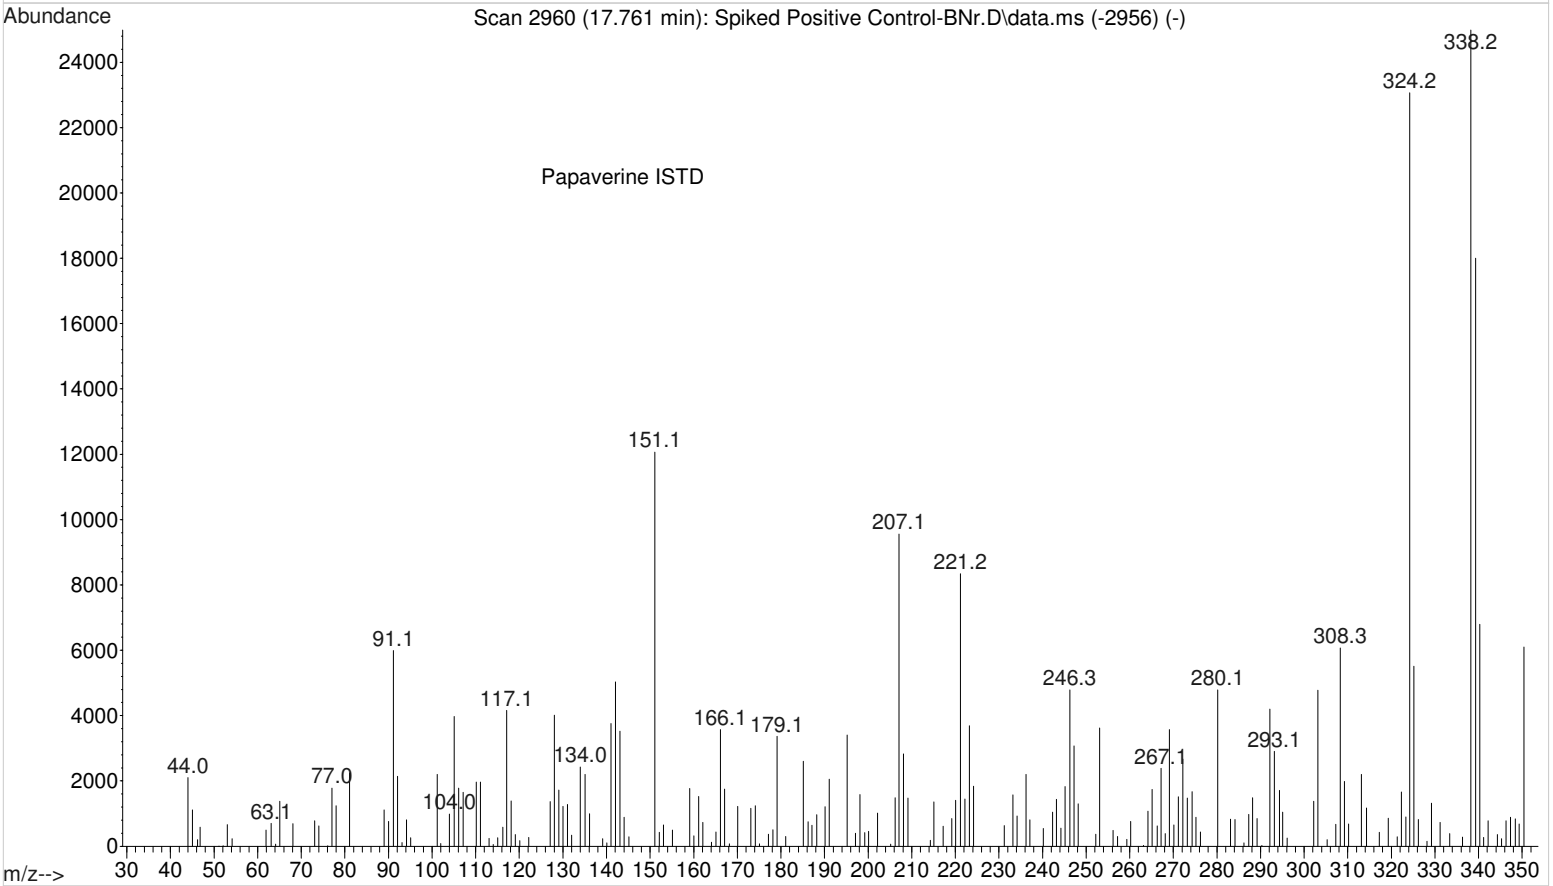

File :I:\Instrument Data\Pocatello\Major Mass Spec\TM\2017\0113201
... 7\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 13 Jan 2017 18:20 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

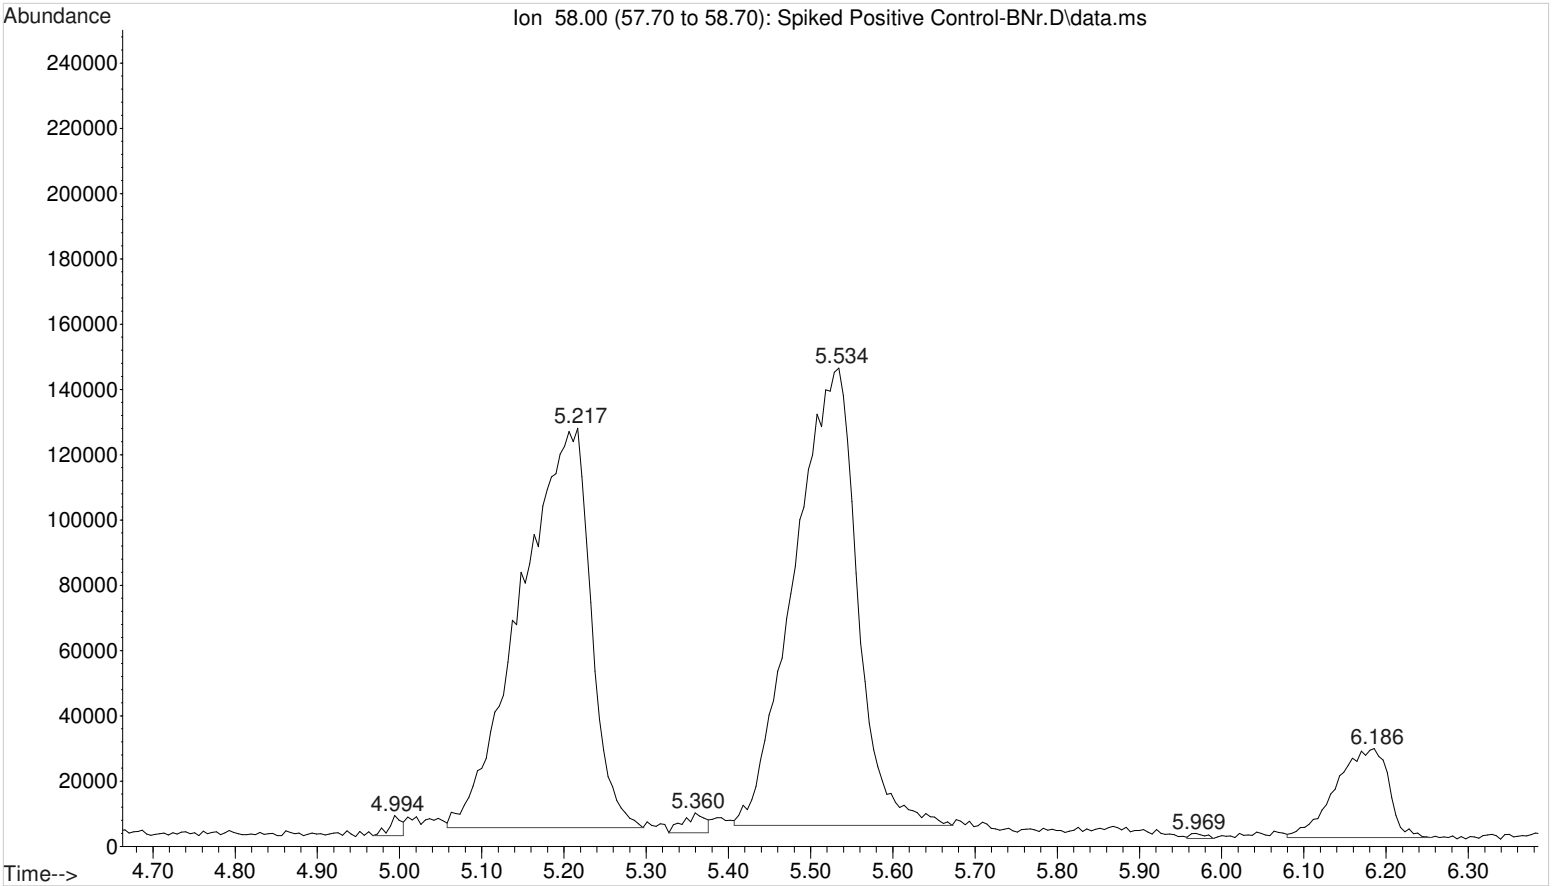

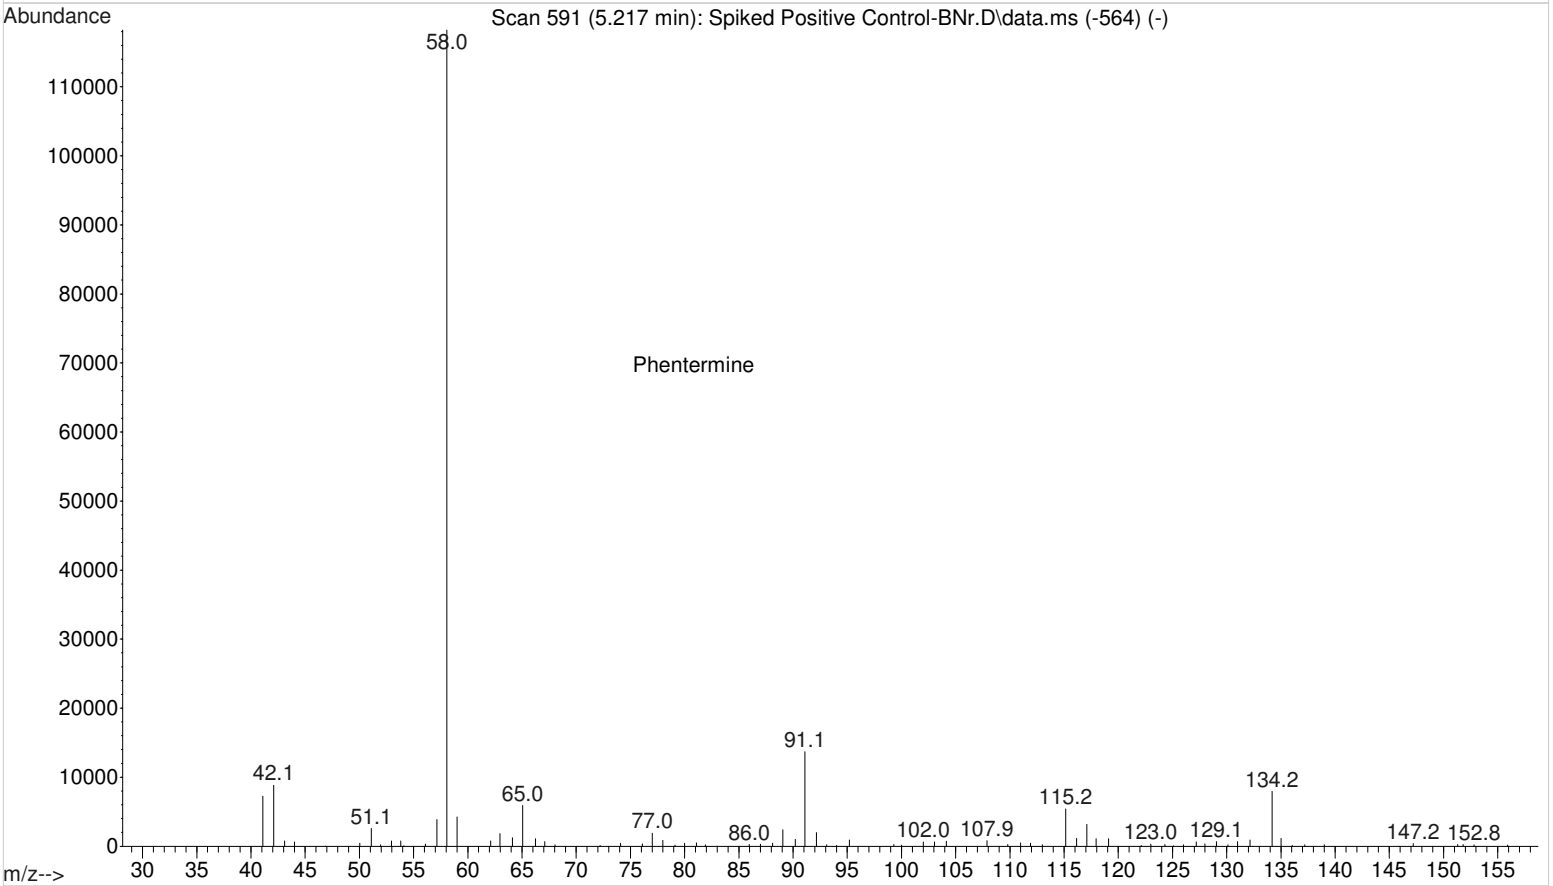

File :I:\Instrument Data\Pocatello\Major Mass Spec\TM\2017\0113201
... 7\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 13 Jan 2017 18:20 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

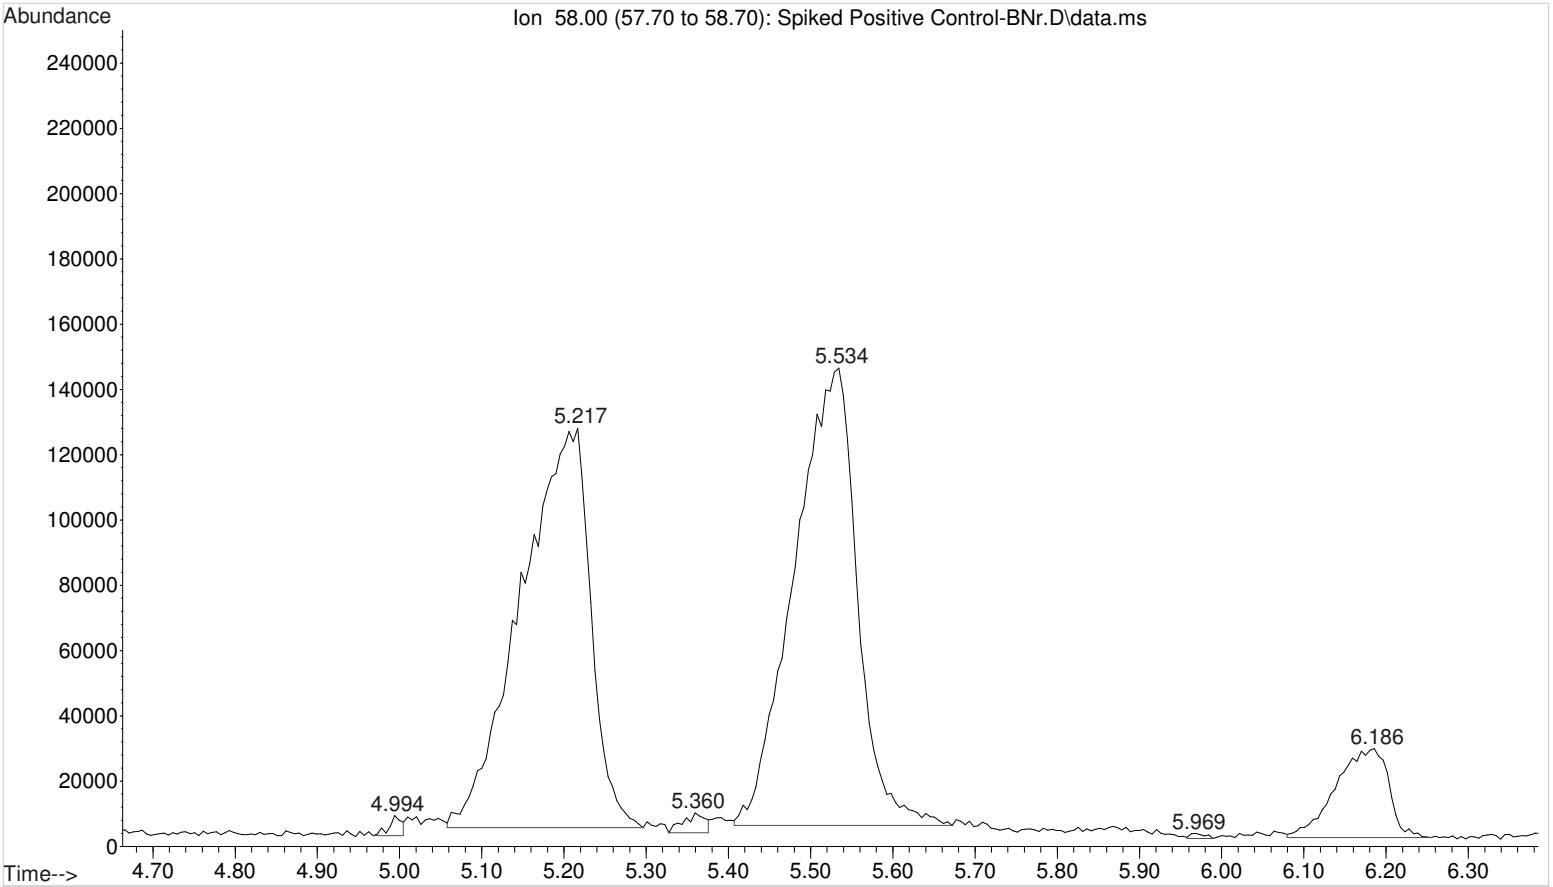

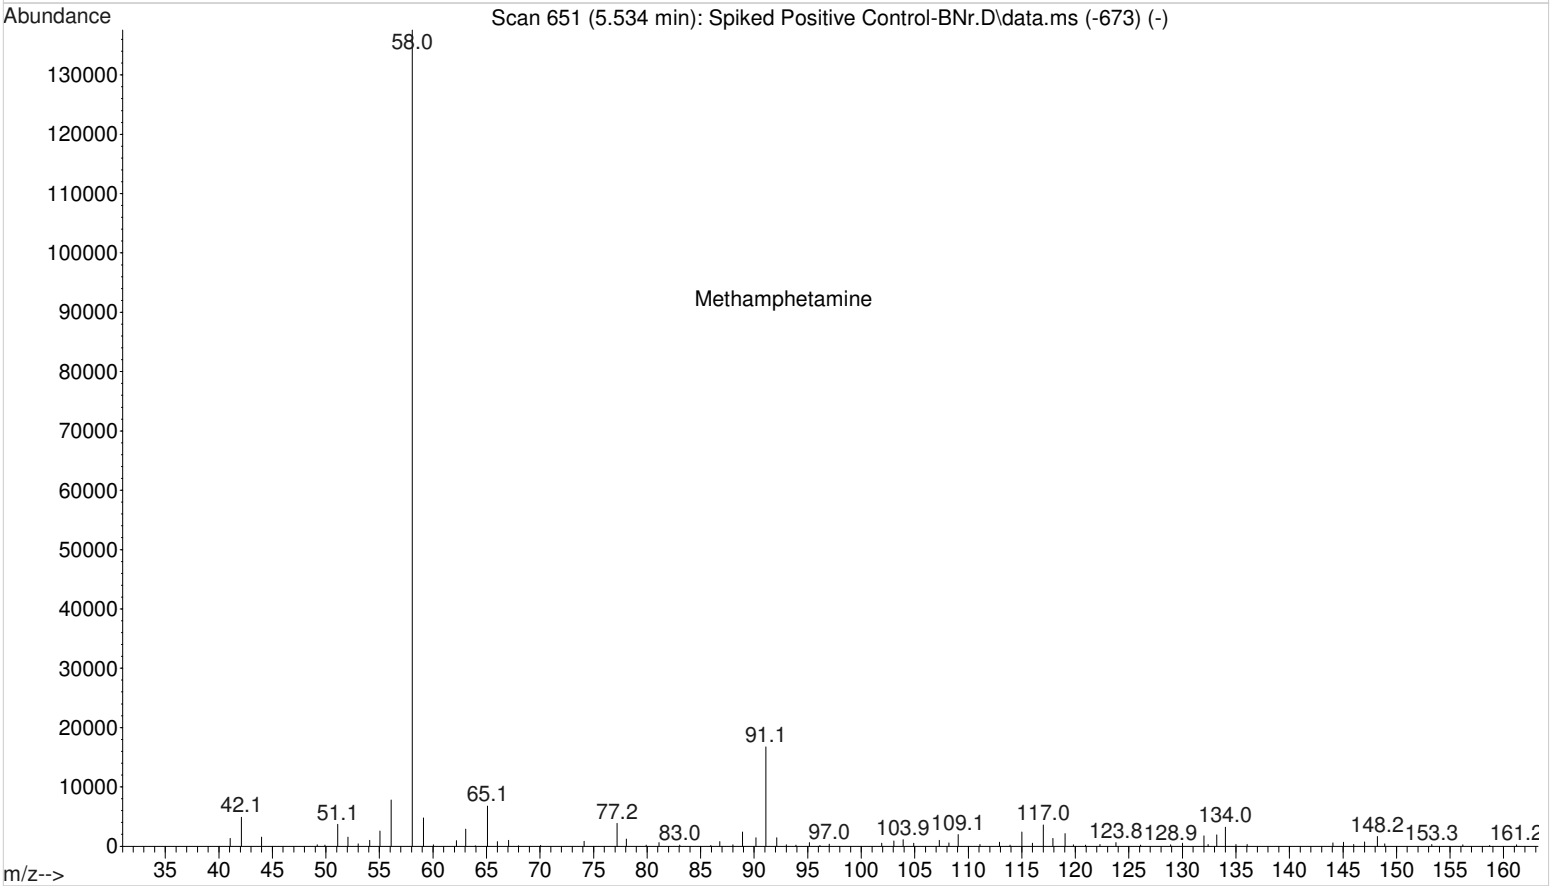

File :I:\Instrument Data\Pocatello\Major Mass Spec\TM\2017\0113201
... 7\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 13 Jan 2017 18:20 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

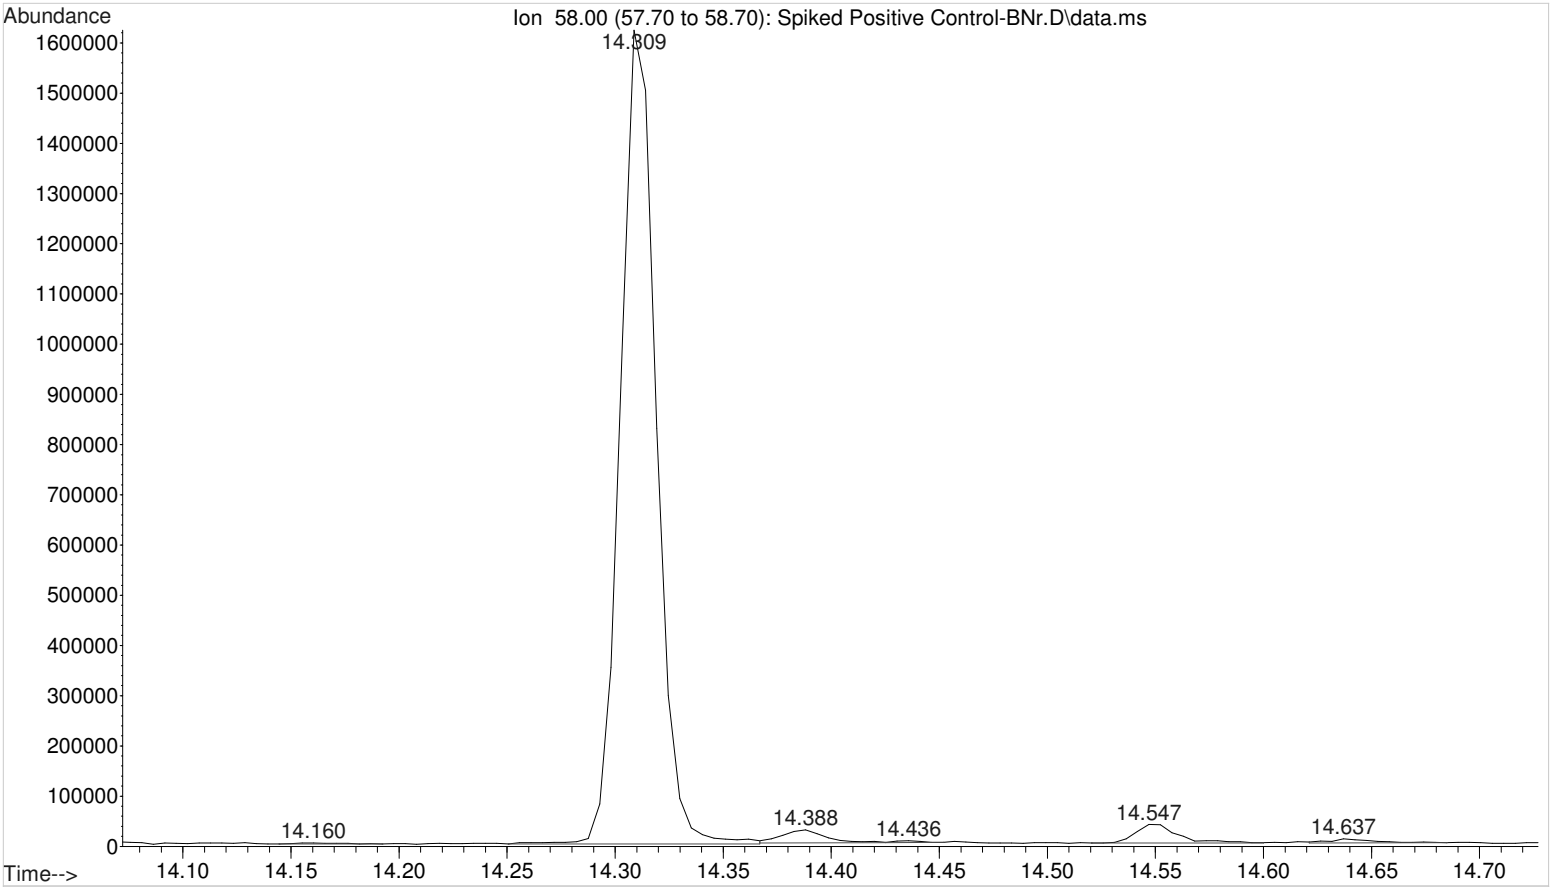

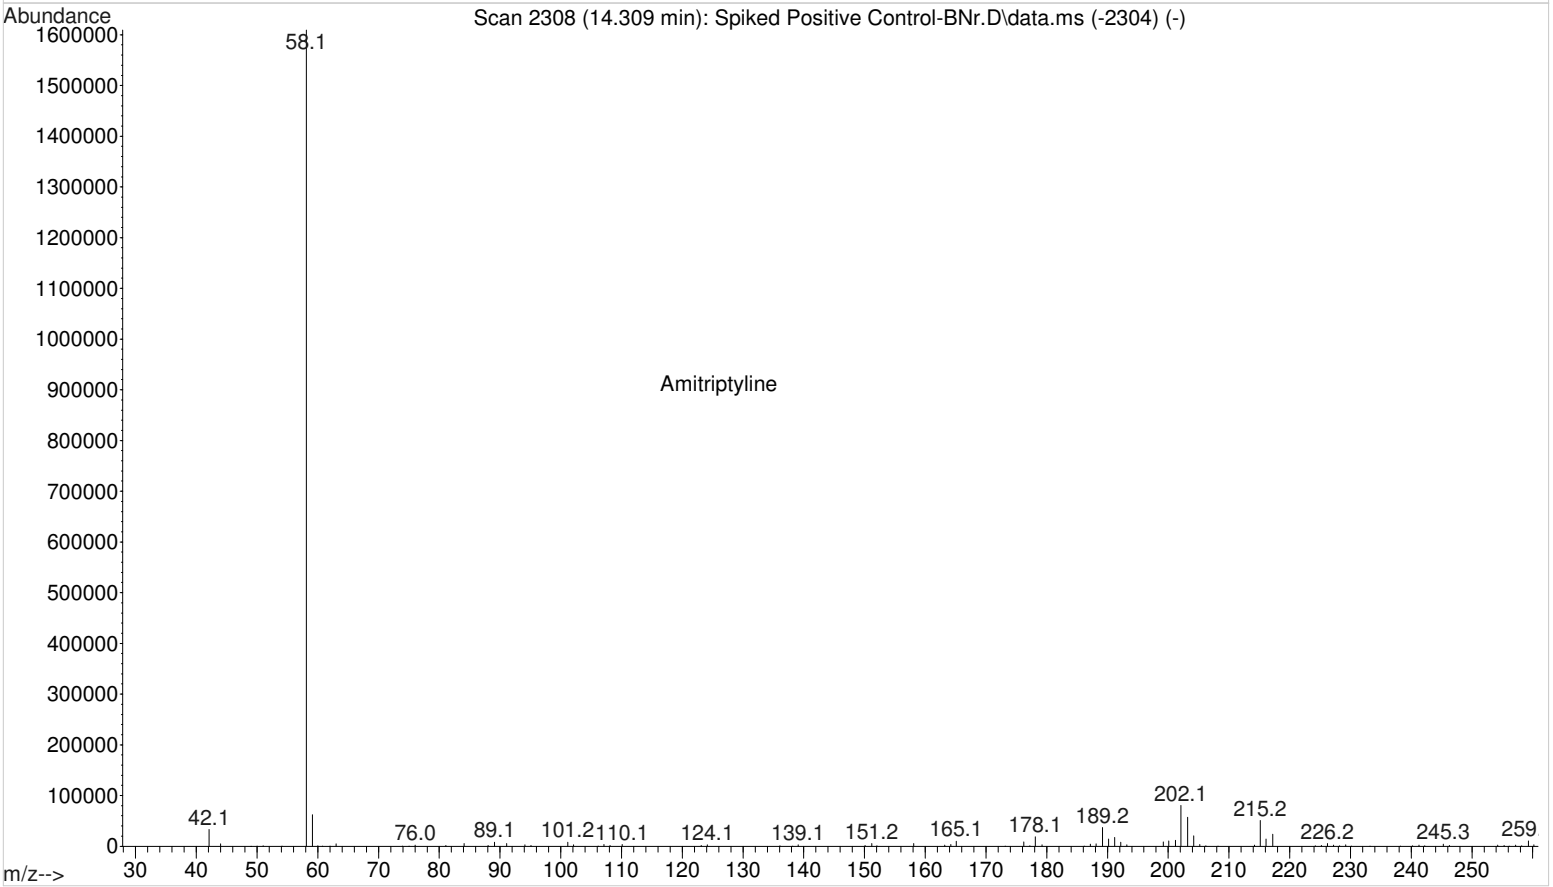

File :I:\Instrument Data\Pocatello\Major Mass Spec\TM\2017\0113201
... 7\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 13 Jan 2017 18:20 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215

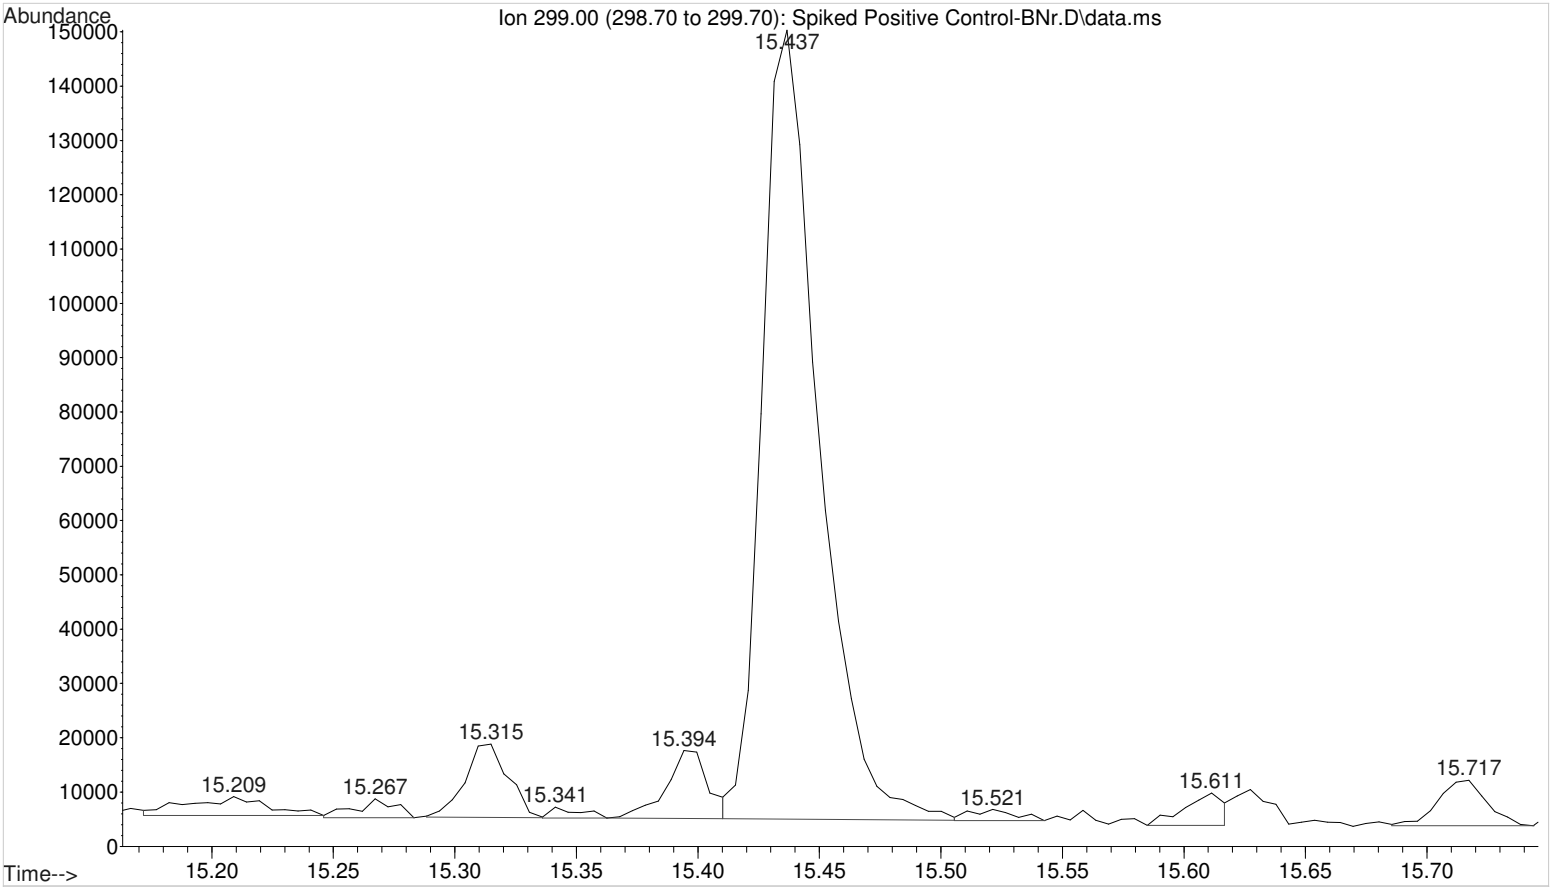

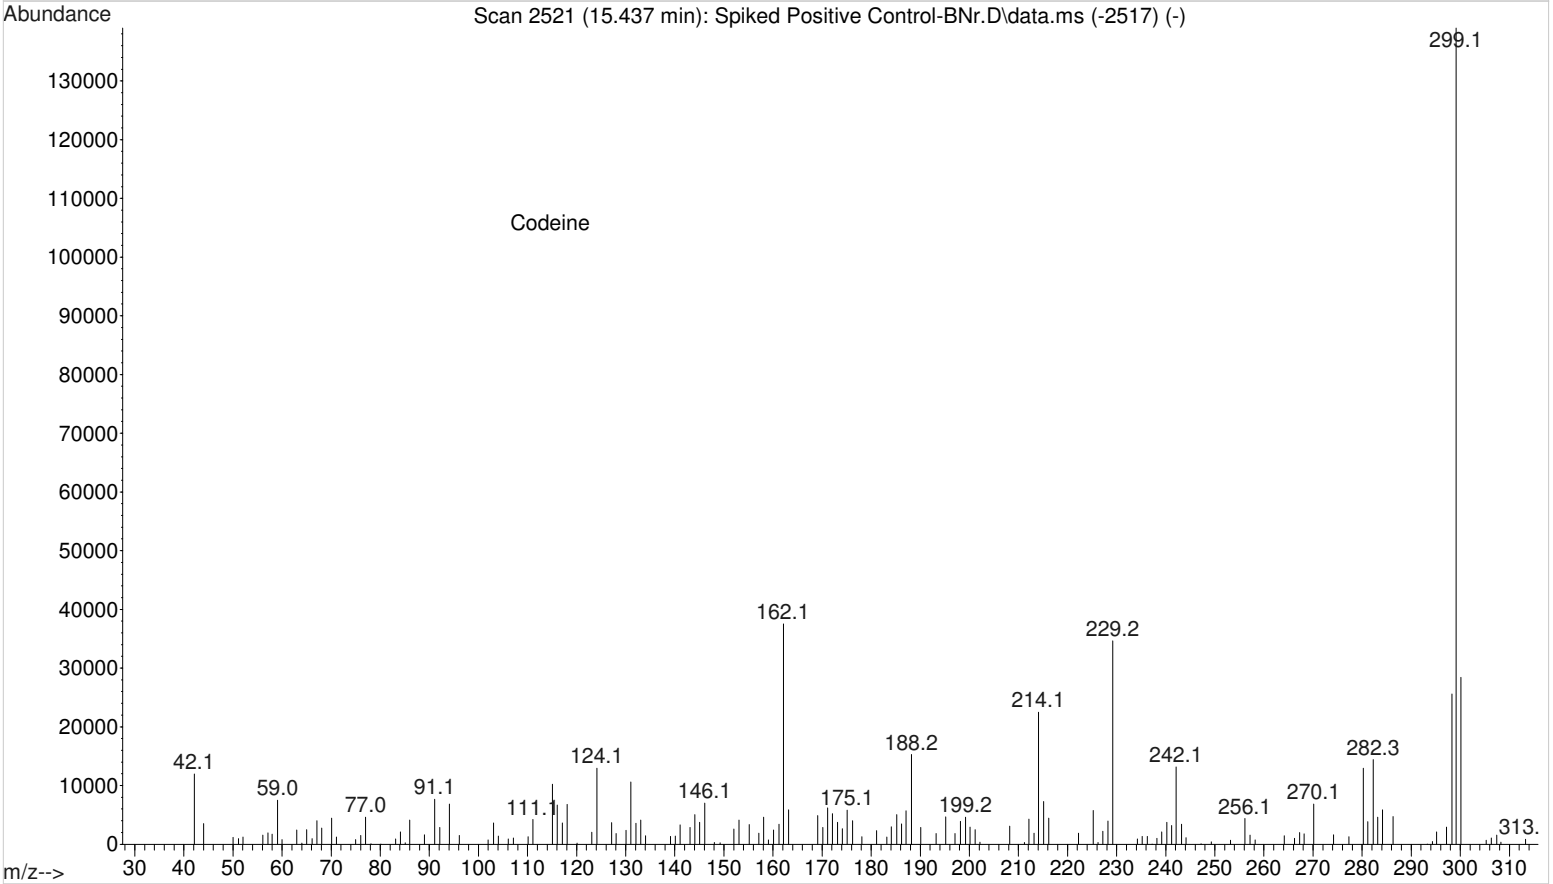

File :I:\Instrument Data\Pocatello\Major Mass Spec\TM\2017\0113201
... 7\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 13 Jan 2017 18:20 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : UTAK B1013 + WS111215