
























**Worklist: 1159**

<u>LAB_CASE</u>	<u>ITEM</u>	<u>TASK_ID</u>	<u>DESCRIPTION</u>	
C2016-0617	1	54464	3.6.1 Blood base neutral confirr	
M2016-0268	2	58197	3.6.1 Blood base neutral confirr	
M2016-0417	1	49965	3.6.1 Blood base neutral confirr	
M2016-0529	1	50482	3.6.1 Blood base neutral confirr	
M2016-0822	2	51985	3.6.1 Blood base neutral confirr	
M2016-0934	2	52394	3.6.1 Blood base neutral confirr	
M2016-1098	1	52997	3.6.1 Blood base neutral confirr	
M2016-1198	1	53481	3.6.1 Blood base neutral confirr	
M2016-1211	1	53534	3.6.1 Blood base neutral confirr	
M2016-1498	1	54709	3.6.1 Blood base neutral confirr	
M2016-1518	1	54752	3.6.1 Blood base neutral confirr	
M2016-1560	1	54888	3.6.1 Blood base neutral confirr	
M2016-1600	1	55022	3.6.1 Blood base neutral confirr	
M2016-1675	1	55402	3.6.1 Blood base neutral confirr	
P2016-0259	1	50112	3.6.1 Blood base neutral confirr	
P2016-0333	1	50798	3.6.1 Blood base neutral confirr	
P2016-0340	1	50821	3.6.1 Blood base neutral confirr	
P2016-0345	1	50854	3.6.1 Blood base neutral confirr	
P2016-0352	1	51001	3.6.1 Blood base neutral confirr	
P2016-0404	1	51311	3.6.1 Blood base neutral confirr	
P2016-0897	1	54670	3.6.1 Blood base neutral confirr	
P2016-0965	1	55106	3.6.1 Blood base neutral confirr	
P2016-1031	1	55515	3.6.1 Blood base neutral confirr	

**Worklist: 1159**

<u>LAB CASE</u>	<u>ITEM</u>	<u>TASK ID</u>	<u>DESCRIPTION</u>
P2016-1053	1	55695	3.6.1 Blood base neutral confirr
P2016-1147	1	56388	3.6.1 Blood base neutral confirr



Reviewed 6/28/16 AMN

A handwritten signature in green ink, consisting of several loops and a long horizontal stroke.

Positive Control = UTAK B1013 + WS111215 ۵

simulate\_sequence.log  
 Simulate Run Sequence Thu Jun 16 12:42:19 2016

Instrument Name: Major Mass Spec  
 Sequence File: C:\Users\ISPuser\Desktop\Sequences\CS-BNSB061616.sequence.xml  
 Comment: MassHunter sequence  
 Operator: ISP\datastor  
 Data Path: D:\DATA\CDS\2016\061616\  
 Method Path: C:\Users\datastor\Desktop\OP Methods\

Line	Type	Vials	DataFile	Sample Name
Acquisition Method: BNSB120510.M				
1)	Sample	100	Prerun Solvent Blank	Pre-run Solvent Blank
2)	Sample	1	Negative Control-BN	Negative Control -
...	1013			
3)	Sample	2	Spiked Positive Control-BN	Positive Control
4)	Sample	99	prBLK2	Solvent Blank
Acquisition Method: GBT092509-Delta EMV.M				
5)	Sample	100	Prerun Solvent Blankr	Pre-run Solvent Blank
6)	Sample	1	Negative Control-BNr	Negative Control -
...	1013			
7)	Sample	2	Spiked Positive Control-BNr	Positive Control
8)	Sample	99	prBLK2r	Solvent Blank
Acquisition Method: BNSB120510.M				
9)	Sample	100	C2016-0617-1-BNBLK	Lab No.: C2016-0617-1
10)	Sample	3	C2016-0617-1-BN	Lab No.: C2016-0617-1
11)	Sample	100	M2016-0268-2-BNBLK	Lab No.: M2016-0268-2
12)	Sample	4	M2016-0268-2-BN	Lab No.: M2016-0268-2
13)	Sample	100	M2016-0417-1-BNBLK	Lab No.: M2016-0417-1
14)	Sample	5	M2016-0417-1-BN	Lab No.: M2016-0417-1
15)	Sample	100	M2016-0529-1-BNBLK	Lab No.: M2016-0529-1
16)	Sample	6	M2016-0529-1-BN	Lab No.: M2016-0529-1
17)	Sample	100	M2016-0822-2-BNBLK	Lab No.: M2016-0822-2
18)	Sample	7	M2016-0822-2-BN	Lab No.: M2016-0822-2
19)	Sample	100	M2016-0934-2-BNBLK	Lab No.: M2016-0934-2
20)	Sample	8	M2016-0934-2-BN	Lab No.: M2016-0934-2
21)	Sample	100	M2016-1098-1-BNBLK	Lab No.: M2016-1098-1
22)	Sample	9	M2016-1098-1-BN	Lab No.: M2016-1098-1
23)	Sample	100	M2016-1198-1-BNBLK	Lab No.: M2016-1198-1
24)	Sample	10	M2016-1198-1-BN	Lab No.: M2016-1198-1
Acquisition Method: GBT092509-Delta EMV.M				
25)	Sample	100	C2016-0617-1-BNBLKr	Lab No.: C2016-0617-1
26)	Sample	3	C2016-0617-1-BNr	Lab No.: C2016-0617-1
27)	Sample	100	M2016-0268-2-BNBLKr	Lab No.: M2016-0268-2
28)	Sample	4	M2016-0268-2-BNr	Lab No.: M2016-0268-2
29)	Sample	100	M2016-0417-1-BNBLKr	Lab No.: M2016-0417-1
30)	Sample	5	M2016-0417-1-BNr	Lab No.: M2016-0417-1
31)	Sample	100	M2016-0529-1-BNBLKr	Lab No.: M2016-0529-1
32)	Sample	6	M2016-0529-1-BNr	Lab No.: M2016-0529-1
33)	Sample	100	M2016-0822-2-BNBLKr	Lab No.: M2016-0822-2
34)	Sample	7	M2016-0822-2-BNr	Lab No.: M2016-0822-2
35)	Sample	100	M2016-0934-2-BNBLKr	Lab No.: M2016-0934-2
36)	Sample	8	M2016-0934-2-BNr	Lab No.: M2016-0934-2
37)	Sample	100	M2016-1098-1-BNBLKr	Lab No.: M2016-1098-1
38)	Sample	9	M2016-1098-1-BNr	Lab No.: M2016-1098-1
39)	Sample	100	M2016-1198-1-BNBLKr	Lab No.: M2016-1198-1
40)	Sample	10	M2016-1198-1-BNr	Lab No.: M2016-1198-1
Acquisition Method: BNSB120510.M				
41)	Sample	100	M2016-1211-1-BNBLK	Lab No.: M2016-1211-1
42)	Sample	11	M2016-1211-1-BN	Lab No.: M2016-1211-1
43)	Sample	100	M2016-1498-1-BNBLK	Lab No.: M2016-1498-1
44)	Sample	12	M2016-1498-1-BN	Lab No.: M2016-1498-1

```

simulate_sequence.log
45) Sample      100      M2016-1518-1-BNBLK      Lab No.: M2016-1518-1
46) Sample      13       M2016-1518-1-BN        Lab No.: M2016-1518-1
47) Sample     100       M2016-1560-1-BNBLK      Lab No.: M2016-1560-1
48) Sample      14       M2016-1560-1-BN        Lab No.: M2016-1560-1
49) Sample     100       M2016-1600-1-BNBLK      Lab No.: M2016-1600-1
50) Sample      15       M2016-1600-1-BN        Lab No.: M2016-1600-1

Acquisition Method: GBT092509-Delta EMV.M
51) Sample     100       M2016-1211-1-BNBLKCr    Lab No.: M2016-1211-1
52) Sample      11       M2016-1211-1-BNr        Lab No.: M2016-1211-1
53) Sample     100       M2016-1498-1-BNBLKCr    Lab No.: M2016-1498-1
54) Sample      12       M2016-1498-1-BNr        Lab No.: M2016-1498-1
55) Sample     100       M2016-1518-1-BNBLKCr    Lab No.: M2016-1518-1
56) Sample      13       M2016-1518-1-BNr        Lab No.: M2016-1518-1
57) Sample     100       M2016-1560-1-BNBLKCr    Lab No.: M2016-1560-1
58) Sample      14       M2016-1560-1-BNr        Lab No.: M2016-1560-1
59) Sample     100       M2016-1600-1-BNBLKCr    Lab No.: M2016-1600-1
60) Sample      15       M2016-1600-1-BNr        Lab No.: M2016-1600-1

Acquisition Method: BNSB120510.M
61) Sample      99       M2016-1675-1-BNBLK      Lab No.: M2016-1675-1
62) Sample      16       M2016-1675-1-BN        Lab No.: M2016-1675-1
63) Sample      99       P2016-0259-1-BNBLK      Lab No.: P2016-0259-1
64) Sample      17       P2016-0259-1-BN        Lab No.: P2016-0259-1
65) Sample      99       P2016-0333-1-BNBLK      Lab No.: P2016-0333-1
66) Sample      18       P2016-0333-1-BN        Lab No.: P2016-0333-1
67) Sample      99       P2016-0340-1-BNBLK      Lab No.: P2016-0340-1
68) Sample      19       P2016-0340-1-BN        Lab No.: P2016-0340-1
69) Sample      99       P2016-0345-1-BNBLK      Lab No.: P2016-0345-1
70) Sample      20       P2016-0345-1-BN        Lab No.: P2016-0345-1

Acquisition Method: GBT092509-Delta EMV.M
71) Sample      99       M2016-1675-1-BNBLKCr    Lab No.: M2016-1675-1
72) Sample      16       M2016-1675-1-BNr        Lab No.: M2016-1675-1
73) Sample      99       P2016-0259-1-BNBLKCr    Lab No.: P2016-0259-1
74) Sample      17       P2016-0259-1-BNr        Lab No.: P2016-0259-1
75) Sample      99       P2016-0333-1-BNBLKCr    Lab No.: P2016-0333-1
76) Sample      18       P2016-0333-1-BNr        Lab No.: P2016-0333-1
77) Sample      99       P2016-0340-1-BNBLKCr    Lab No.: P2016-0340-1
78) Sample      19       P2016-0340-1-BNr        Lab No.: P2016-0340-1
79) Sample      99       P2016-0345-1-BNBLKCr    Lab No.: P2016-0345-1
80) Sample      20       P2016-0345-1-BNr        Lab No.: P2016-0345-1

Acquisition Method: BNSB120510.M
81) Sample      99       P2016-0352-1-BNBLK      Lab No.: P2016-0352-1
82) Sample      21       P2016-0352-1-BN        Lab No.: P2016-0352-1
83) Sample      99       P2016-0404-1-BNBLK      Lab No.: P2016-0404-1
84) Sample      22       P2016-0404-1-BN        Lab No.: P2016-0404-1
85) Sample      99       P2016-0897-1-BNBLK      Lab No.: P2016-0897-1
86) Sample      23       P2016-0897-1-BN        Lab No.: P2016-0897-1
87) Sample      99       P2016-0965-1-BNBLK      Lab No.: P2016-0965-1
88) Sample      24       P2016-0965-1-BN        Lab No.: P2016-0965-1
89) Sample      99       P2016-1031-1-BNBLK      Lab No.: P2016-1031-1
90) Sample      25       P2016-1031-1-BN        Lab No.: P2016-1031-1

Acquisition Method: GBT092509-Delta EMV.M
91) Sample      99       P2016-0352-1-BNBLKCr    Lab No.: P2016-0352-1
92) Sample      21       P2016-0352-1-BNr        Lab No.: P2016-0352-1
93) Sample      99       P2016-0404-1-BNBLKCr    Lab No.: P2016-0404-1
94) Sample      22       P2016-0404-1-BNr        Lab No.: P2016-0404-1
95) Sample      99       P2016-0897-1-BNBLKCr    Lab No.: P2016-0897-1
96) Sample      23       P2016-0897-1-BNr        Lab No.: P2016-0897-1
97) Sample      99       P2016-0965-1-BNBLKCr    Lab No.: P2016-0965-1
98) Sample      24       P2016-0965-1-BNr        Lab No.: P2016-0965-1
99) Sample      99       P2016-1031-1-BNBLKCr    Lab No.: P2016-1031-1
100) Sample     25       P2016-1031-1-BNr        Lab No.: P2016-1031-1

Acquisition Method: BNSB120510.M

```

```

simulate_sequence.log
101) Sample          99      P2016-1053-1-BNBLK      Lab No.: P2016-1053-1
102) Sample          26      P2016-1053-1-BN        Lab No.: P2016-1053-1

Acquisition Method: GBT092509-Delta EMV.M
103) Sample          99      P2016-1053-1-BNBLKr    Lab No.: P2016-1053-1
104) Sample          26      P2016-1053-1-BNr       Lab No.: P2016-1053-1

Acquisition Method: BNSB120510.M
105) Sample          99      P2016-1147-1-BNBLK     Lab No.: P2016-1147-1
106) Sample          27      P2016-1147-1-BN        Lab No.: P2016-1147-1

Acquisition Method: GBT092509-Delta EMV.M
107) Sample          99      P2016-1147-1-BNBLKr    Lab No.: P2016-1147-1
108) Sample          27      P2016-1147-1-BNr       Lab No.: P2016-1147-1

Acquisition Method: BNSB120510.M
109) Sample          99      POSTBLK                 BLK

Acquisition Method: GBT092509-Delta EMV.M
110) Sample          99      AFTER                   BLK
megabytes Needed: 2339  Space on drive D: 239253
Sequence Verification Done!

```

Analytical Method 3.6.1 & 3.6.7 QA Check List

---

Run Start Date: 06/16/2016

Analyst: CS

(Short GC/MS temperature program)

Positive Control Compound List


- Phentermine
- Methamphetamine
- Nicotine
- Meperidine
- Caffeine
- Diphenhydramine
- Lidocaine
- PCP
- Methadone
- Amitriptyline
- Codeine
- Trazodone

Internal Standards


- Benzphetamine
- Papaverine

Optional back extraction **not** performed.  
Reconstituted in MeOH.

File :I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Prerun Solvent Blank.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 12:48 using AcqMethod BNSB120510.M  
Sample Name: Pre-run Solvent Blank  
Misc Info : Chloroform

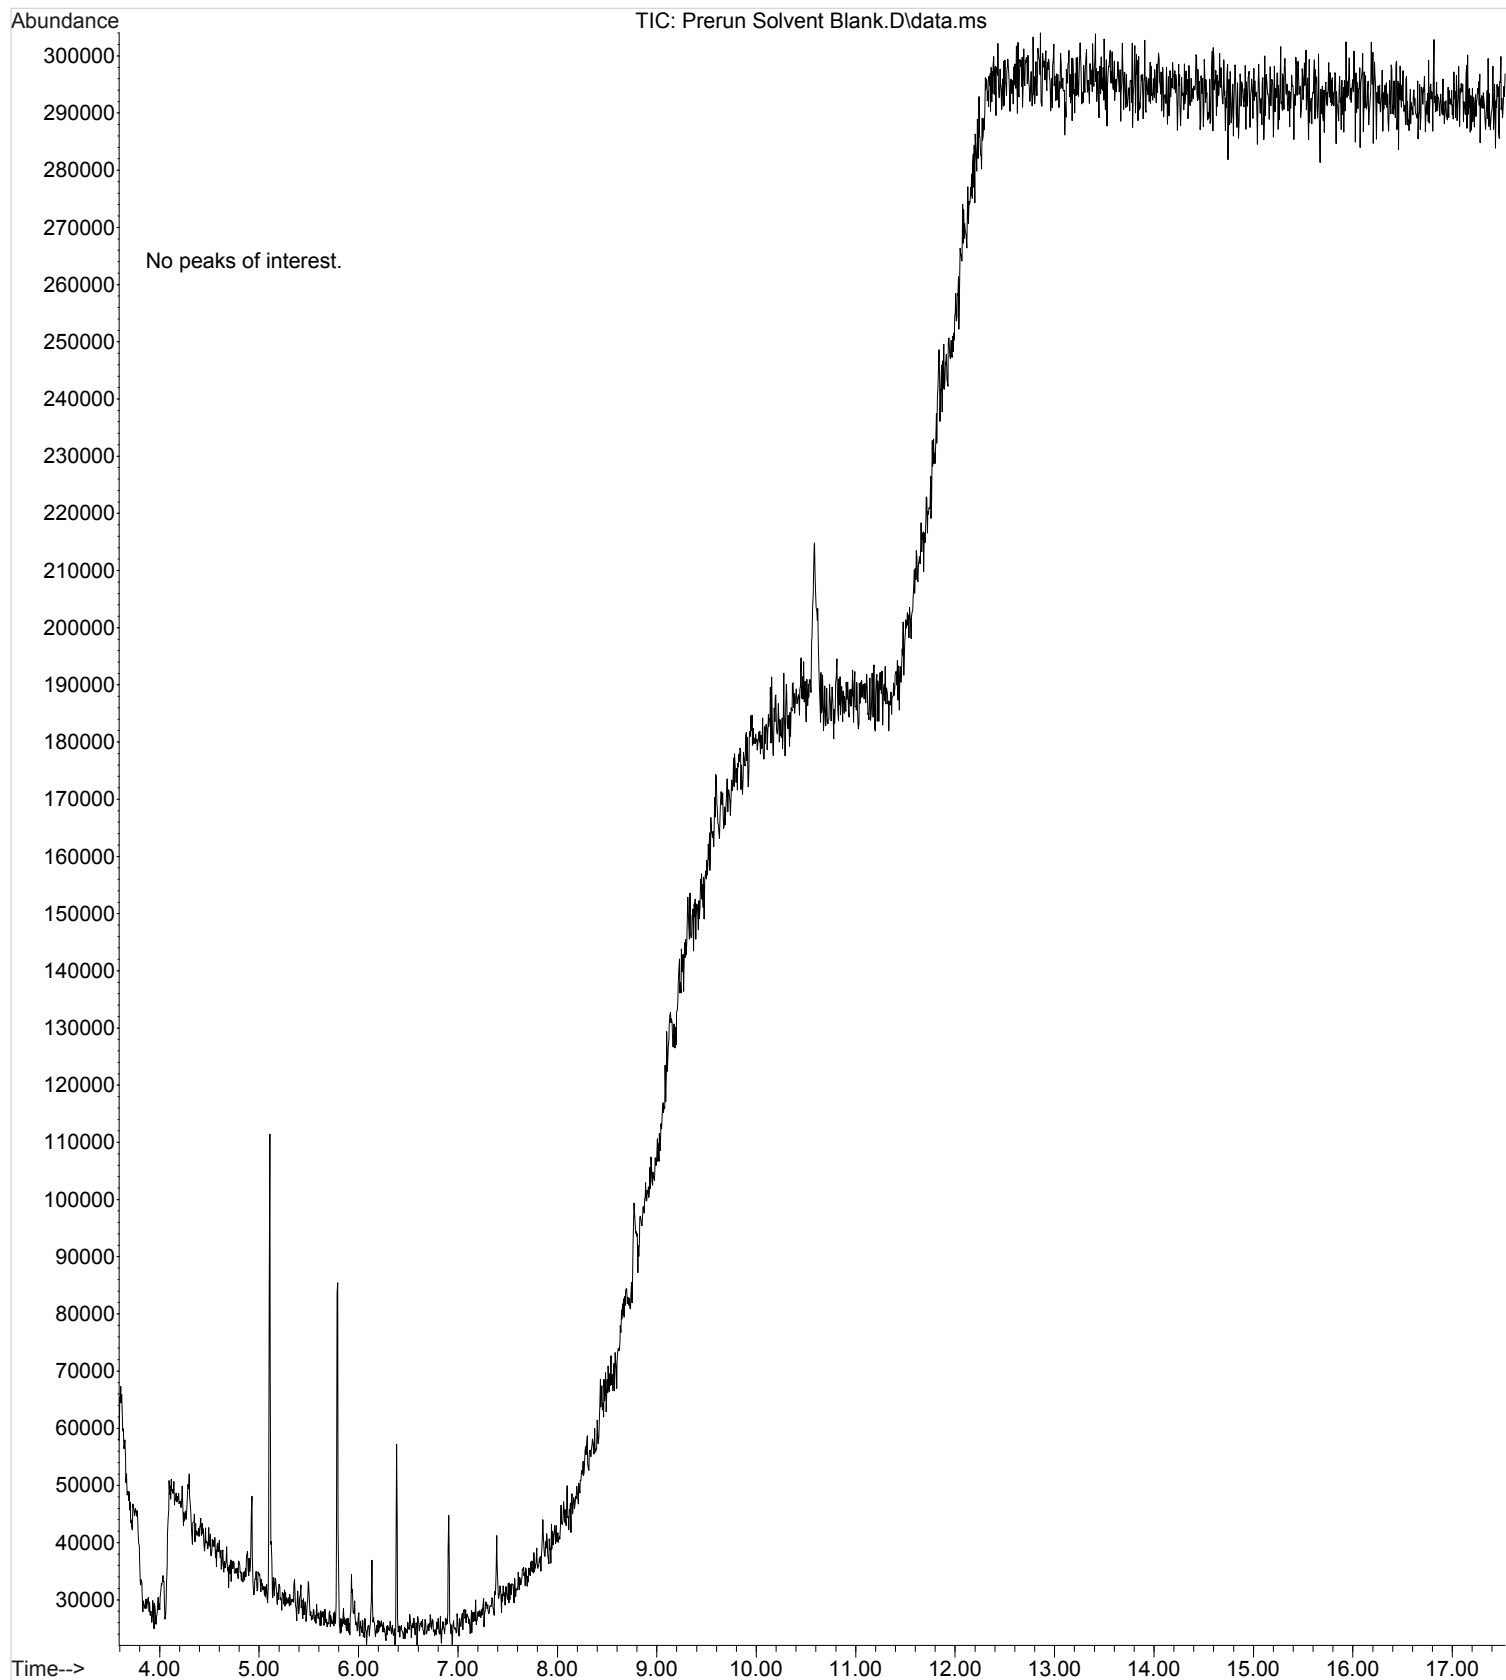


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \prbLK2.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 13:57 using AcqMethod BNSB120510.M  
Sample Name: Solvent Blank  
Misc Info : Chloroform


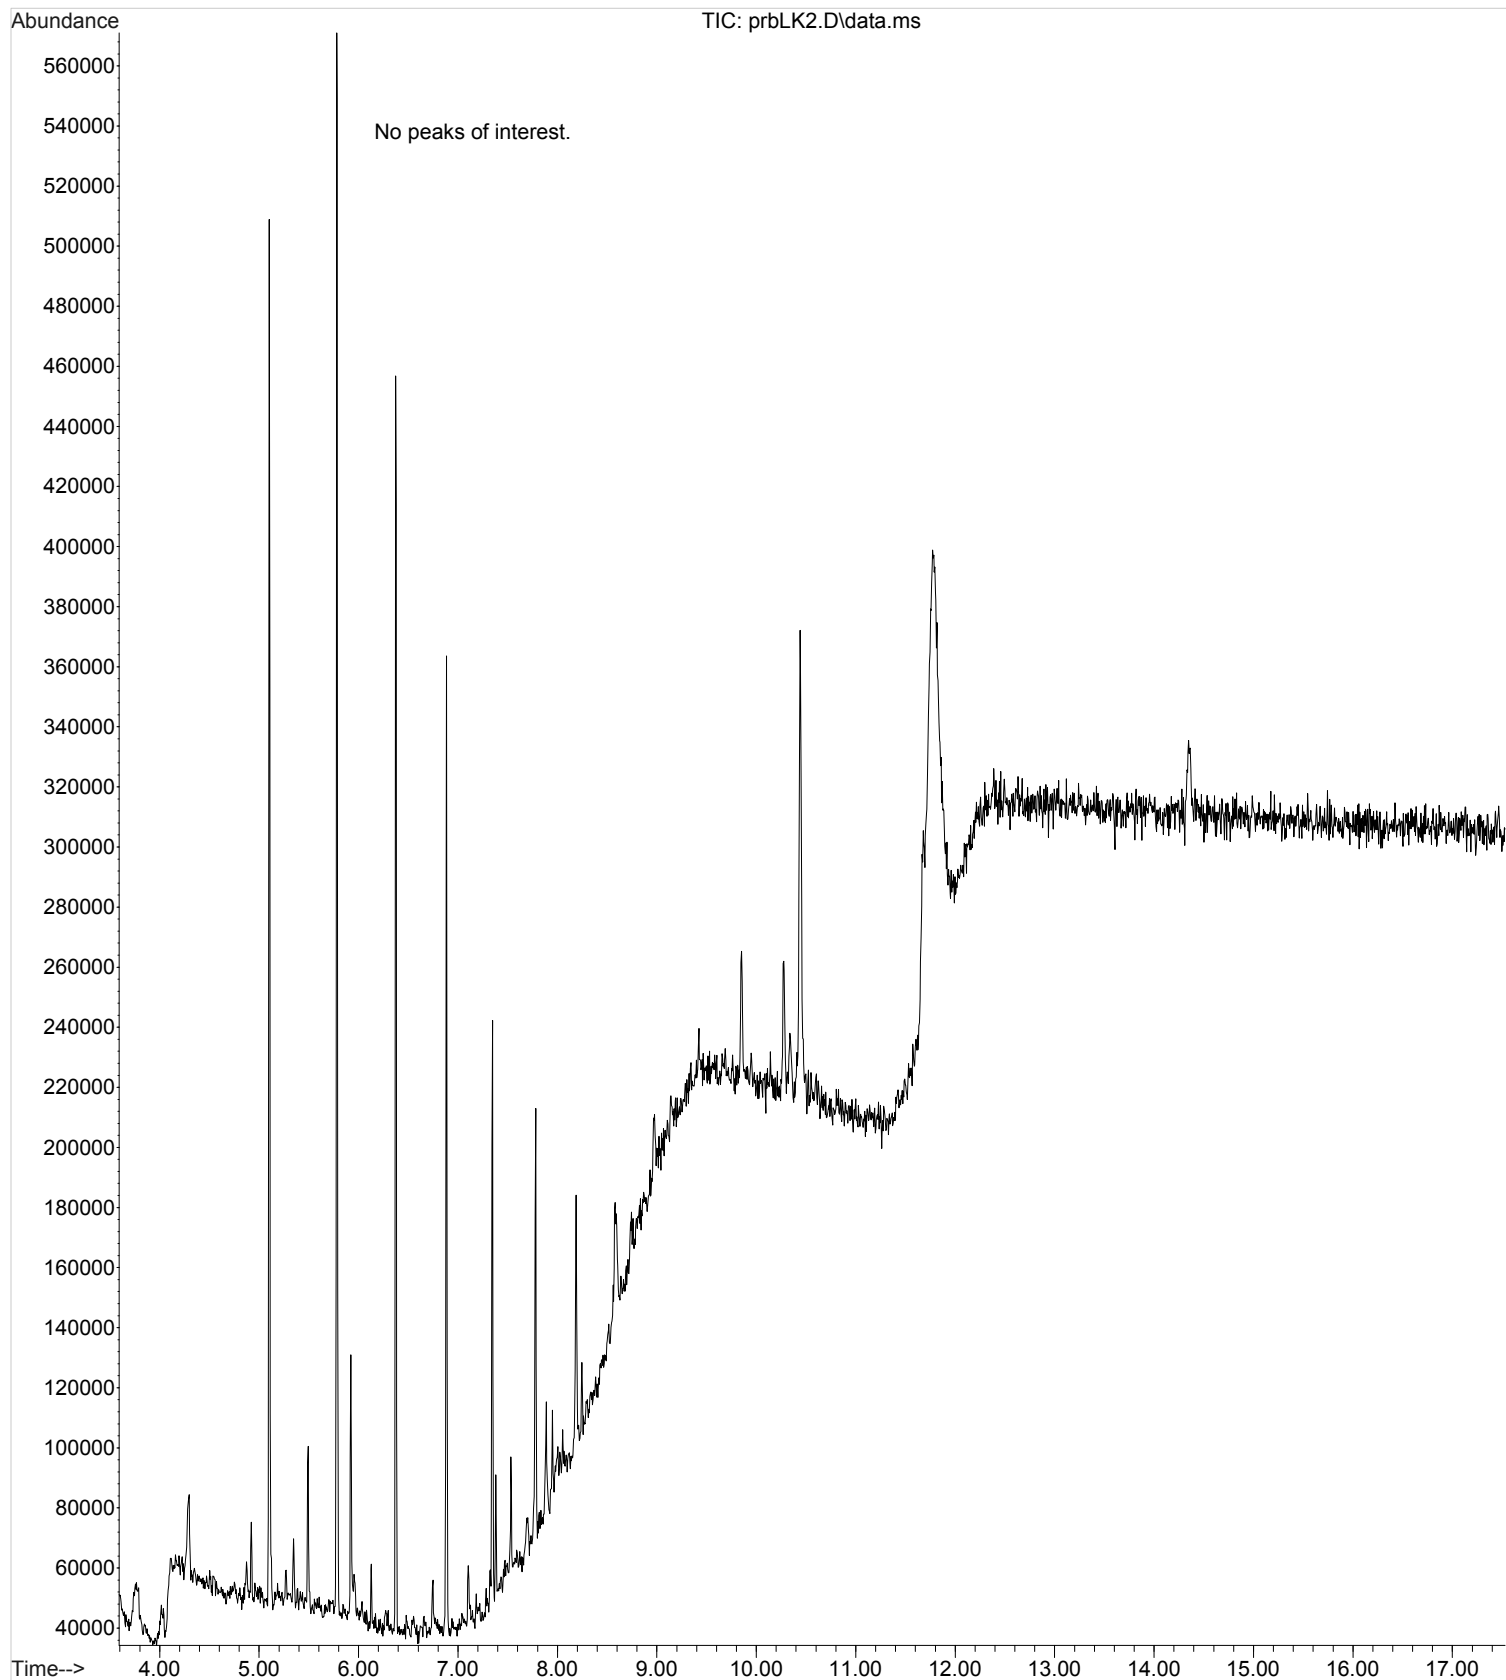






File :I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Negative Control-BN.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 13:11 using AcqMethod BNSB120510.M  
Sample Name: Negative Control - Utak Lot B1013  
Misc Info : Analytical Method 3.6.1

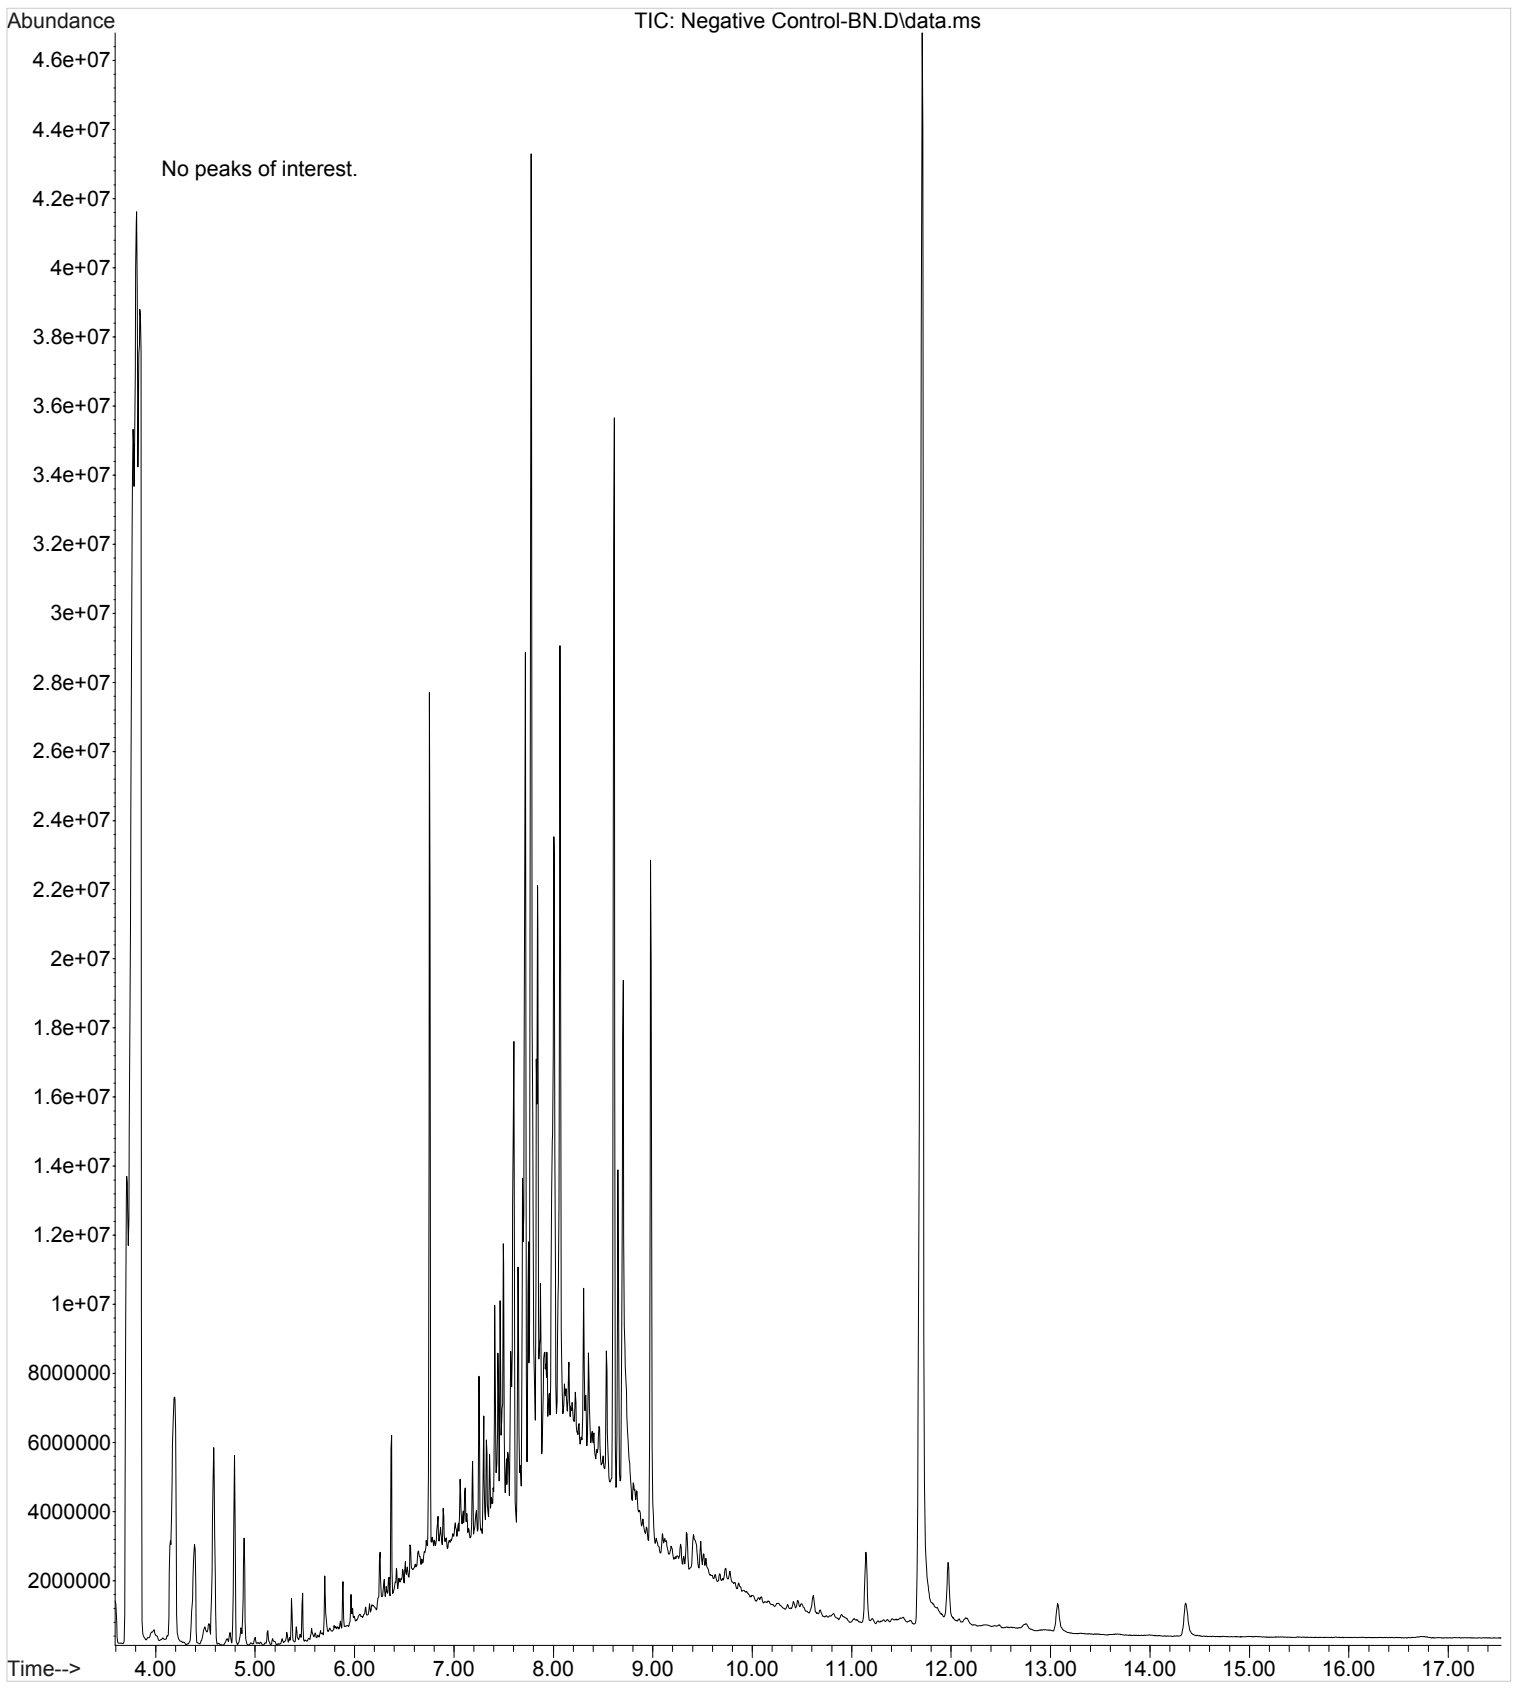


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Negative Control-BN.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 13:11 using AcqMethod BNSB120510.M  
Sample Name: Negative Control - Utak Lot B1013  
Misc Info : Analytical Method 3.6.1

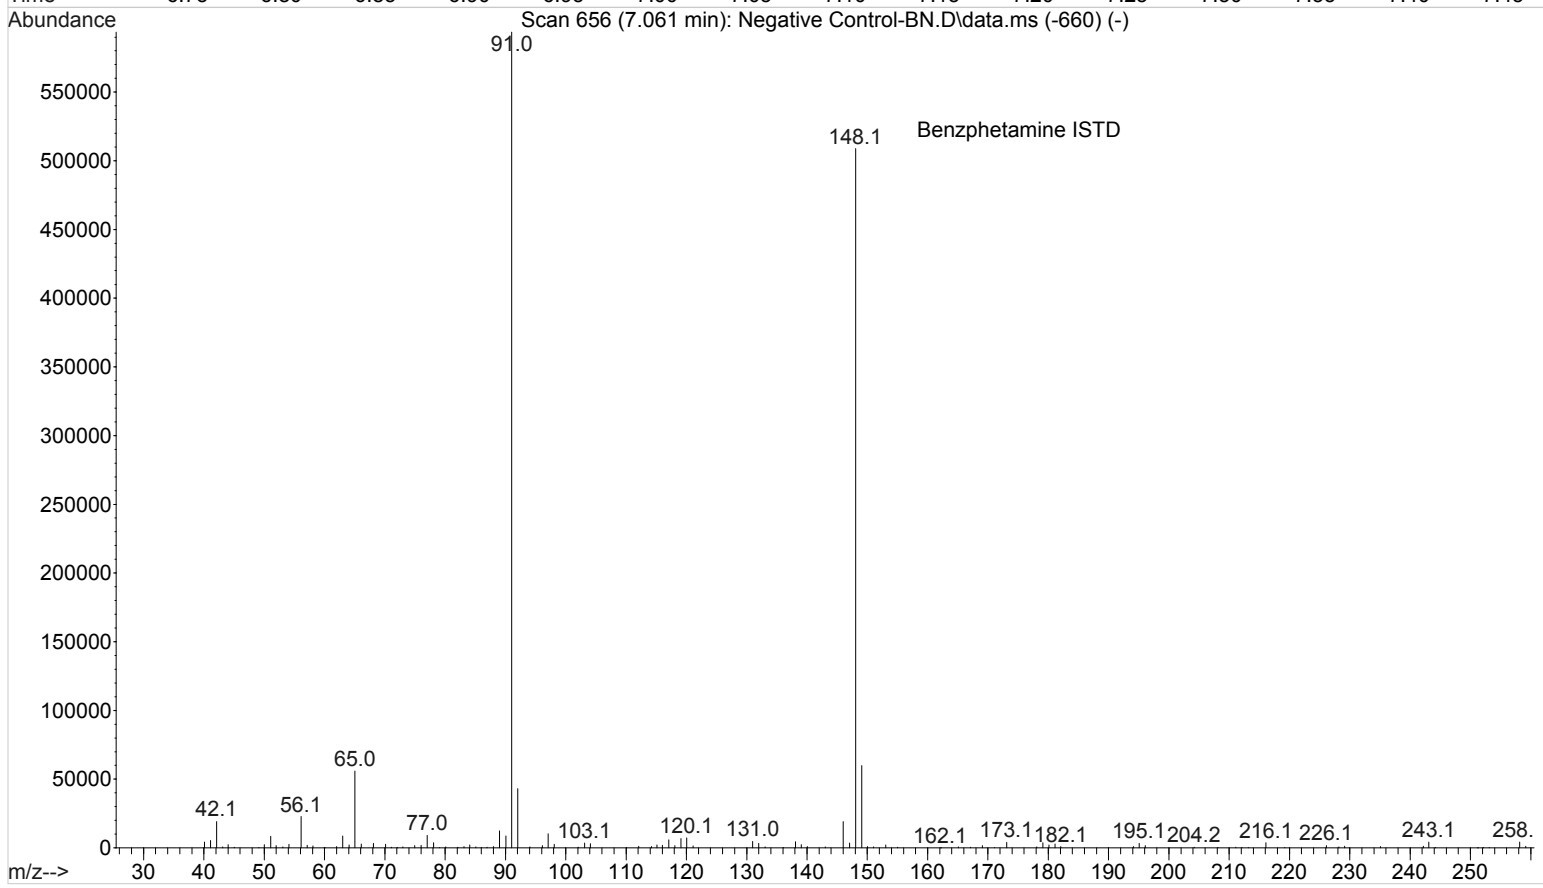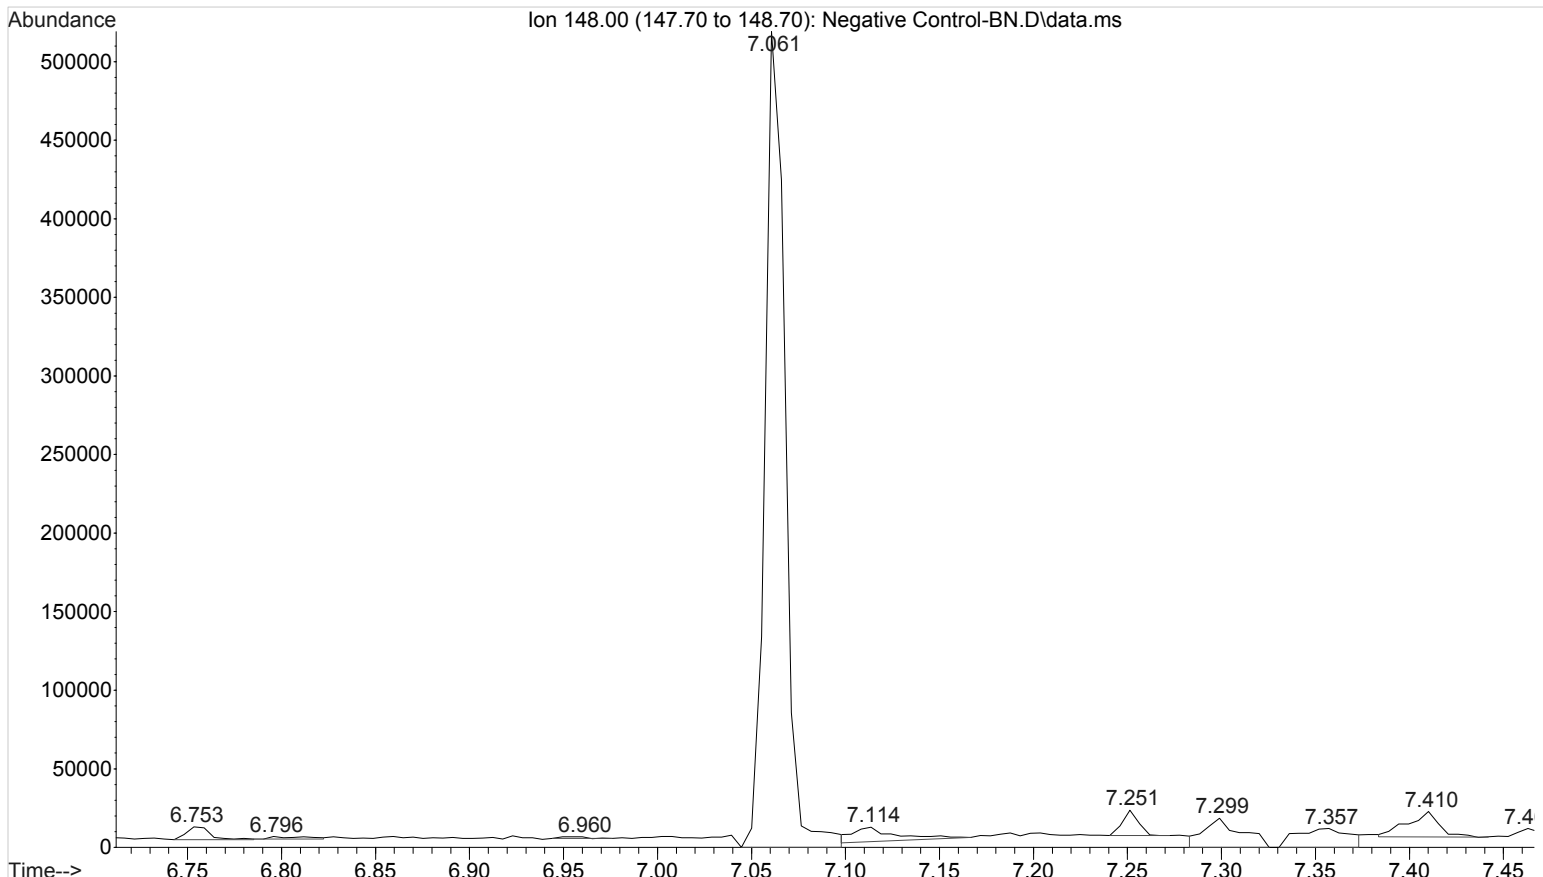

File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Negative Control-BN.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 13:11 using AcqMethod BNSB120510.M  
Sample Name: Negative Control - Utak Lot B1013  
Misc Info : Analytical Method 3.6.1

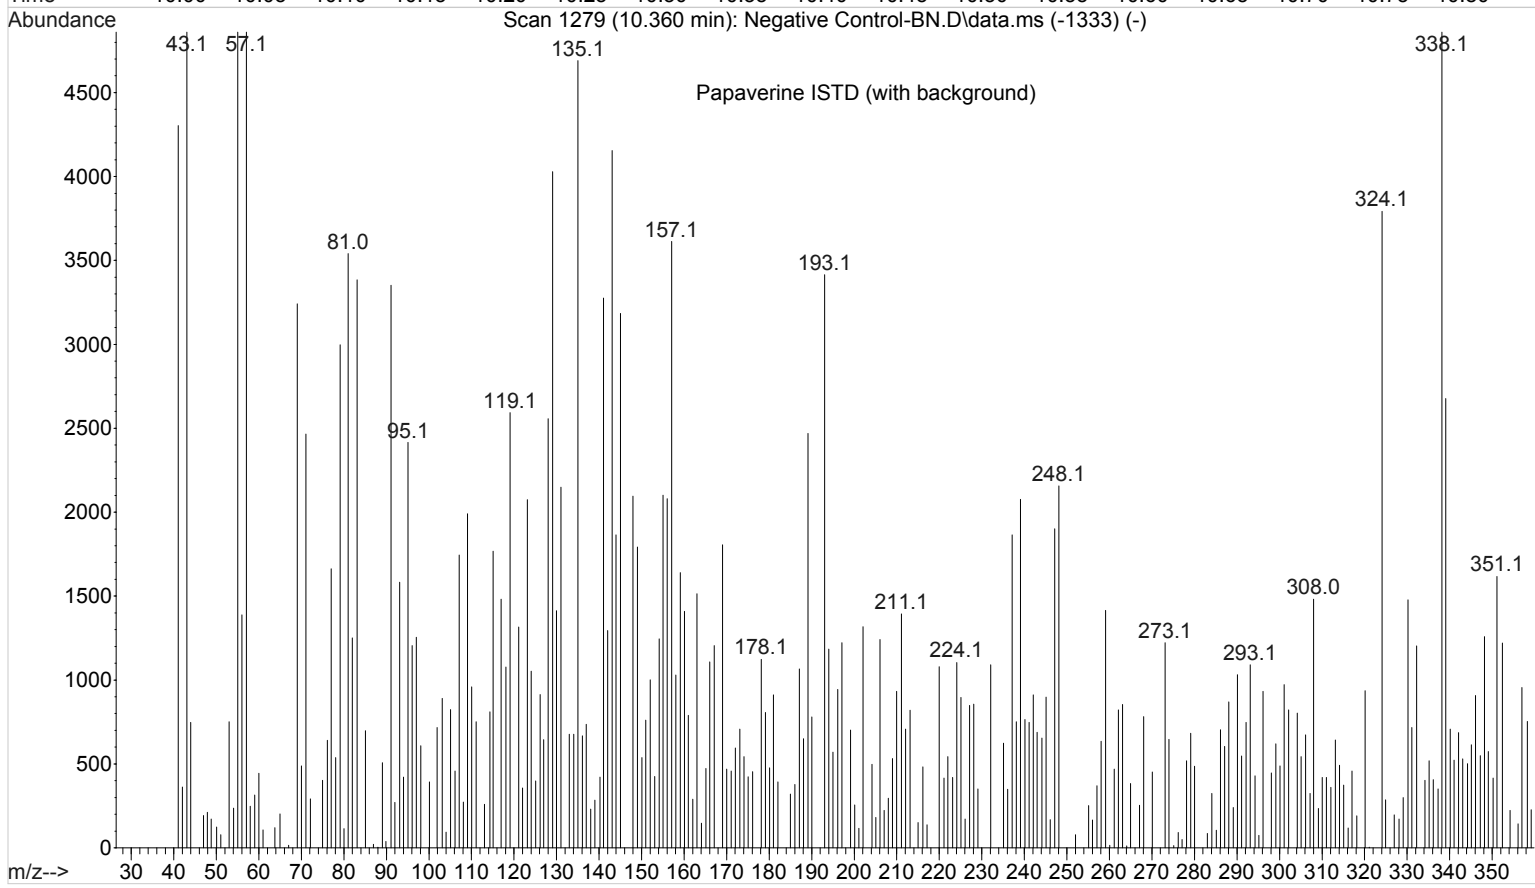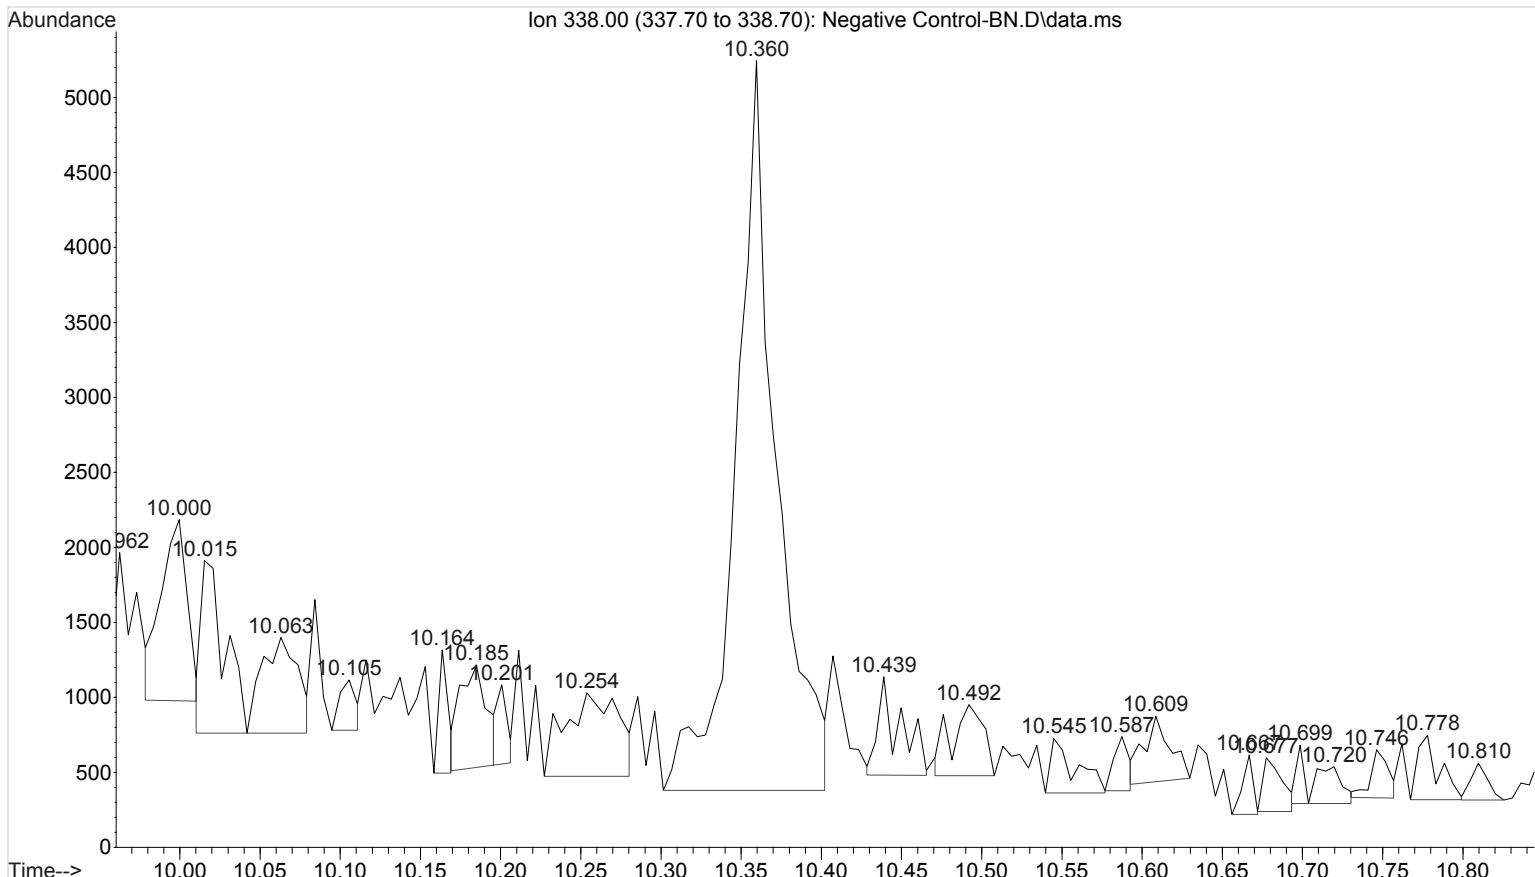


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Spiked Positive Control-BN.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 13:34 using AcqMethod BNSB120510.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215


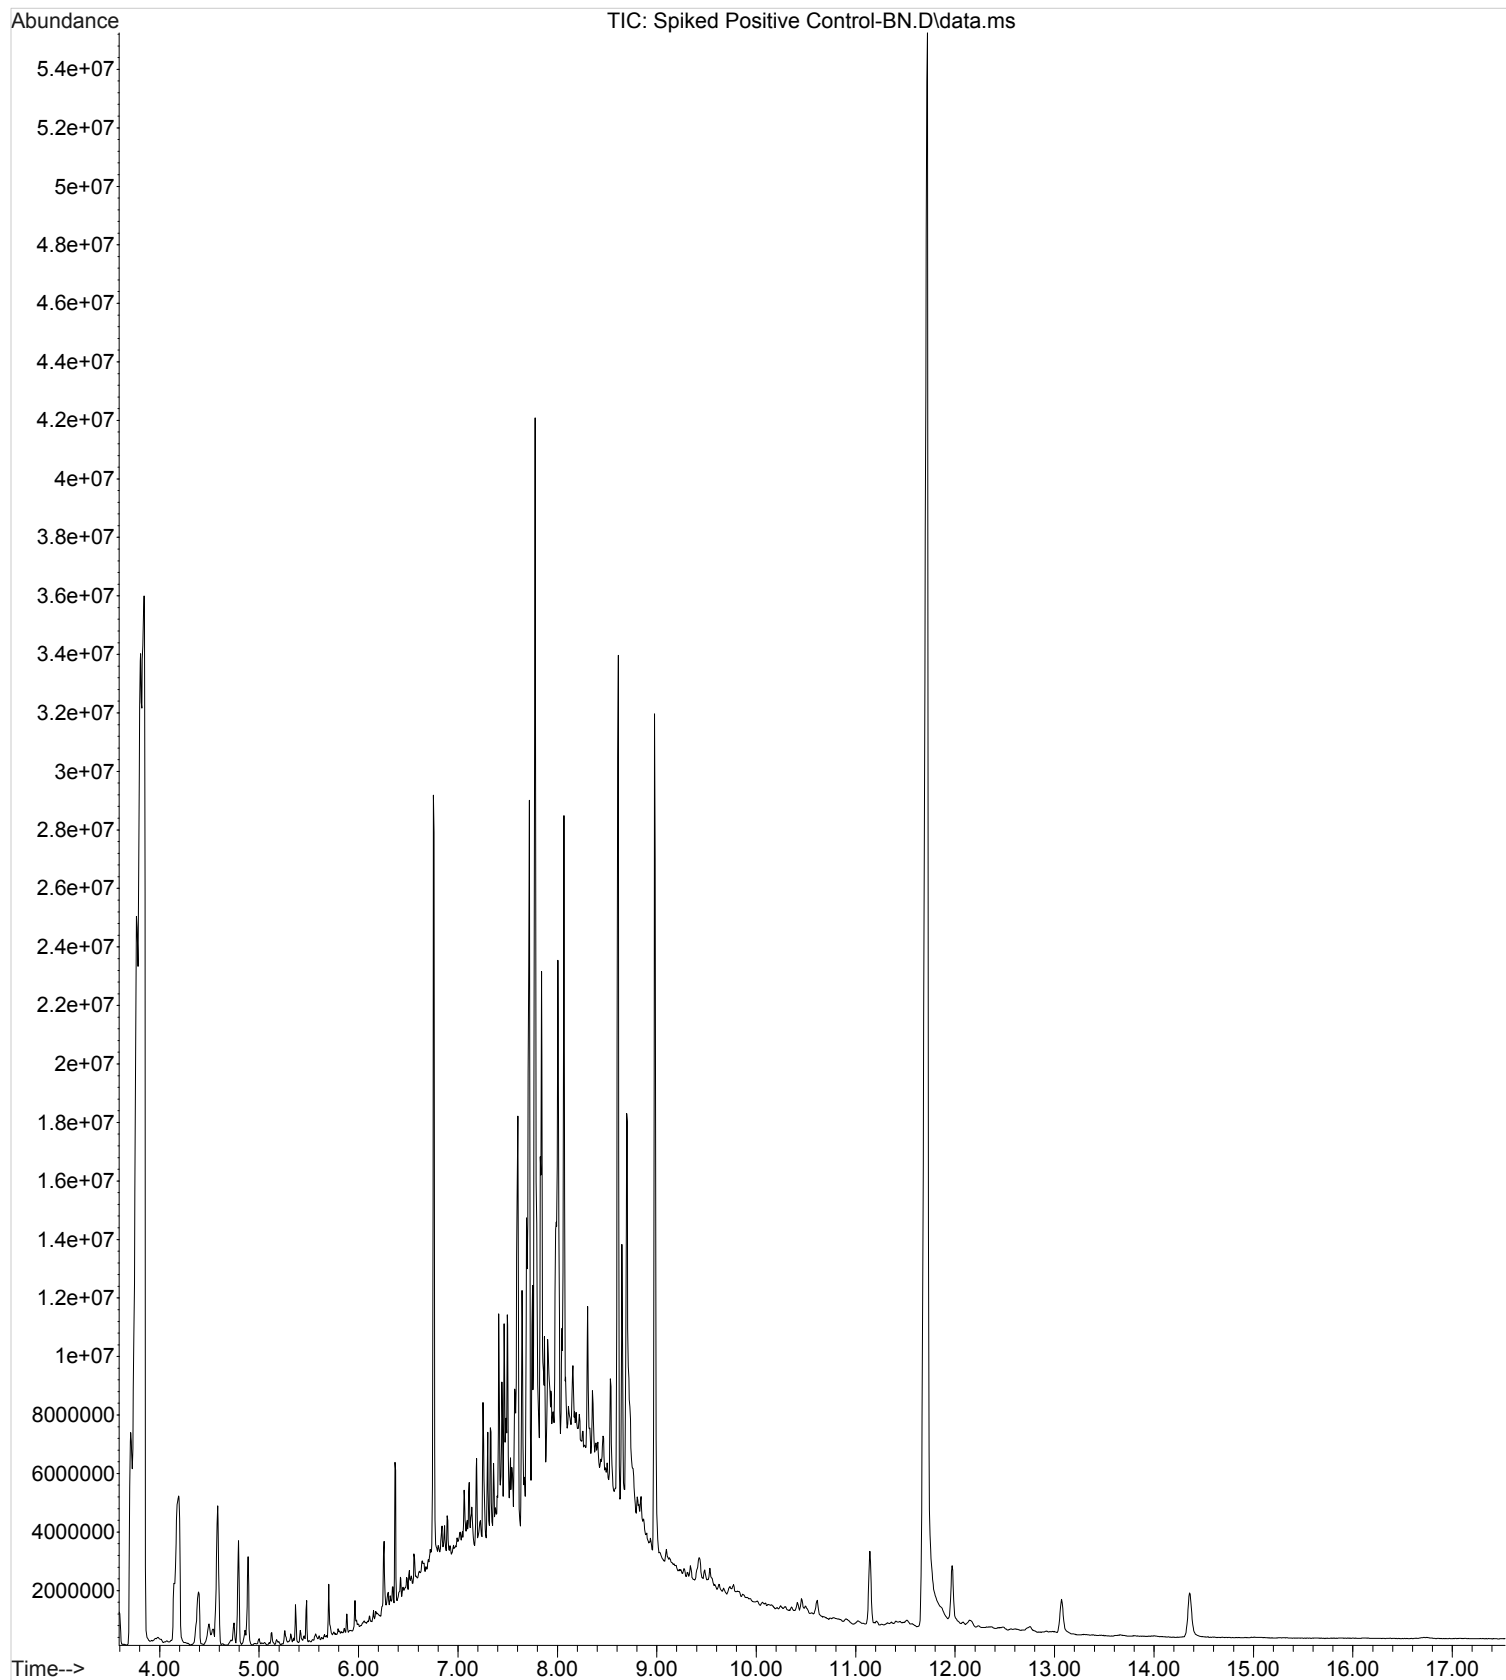


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Spiked Positive Control-BN.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 13:34 using AcqMethod BNSB120510.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215



CS

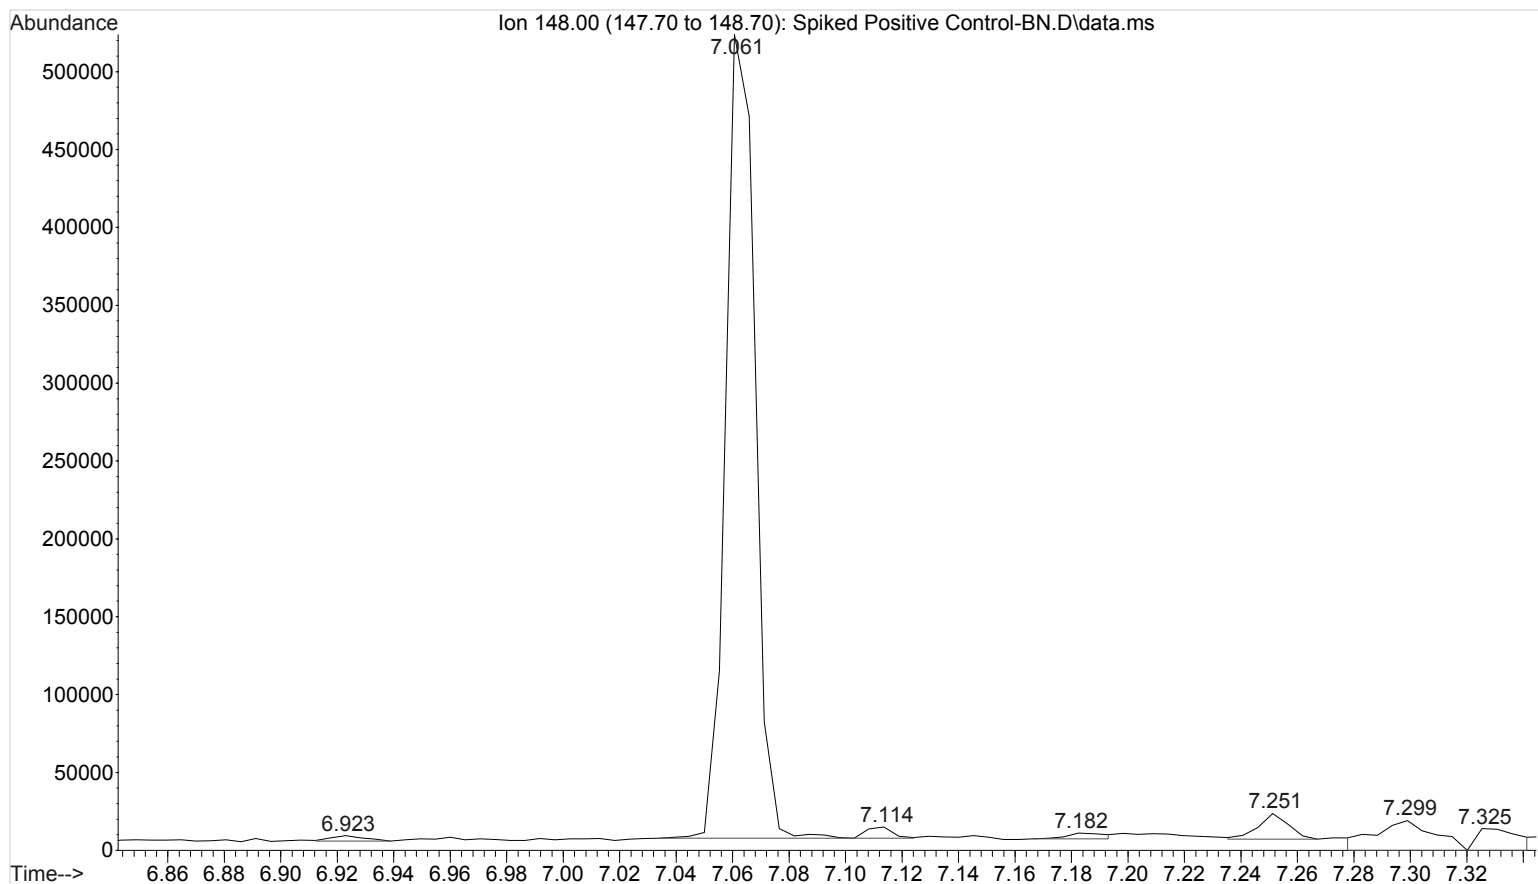

File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Spiked Positive Control-BN.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 13:34 using AcqMethod BNSB120510.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

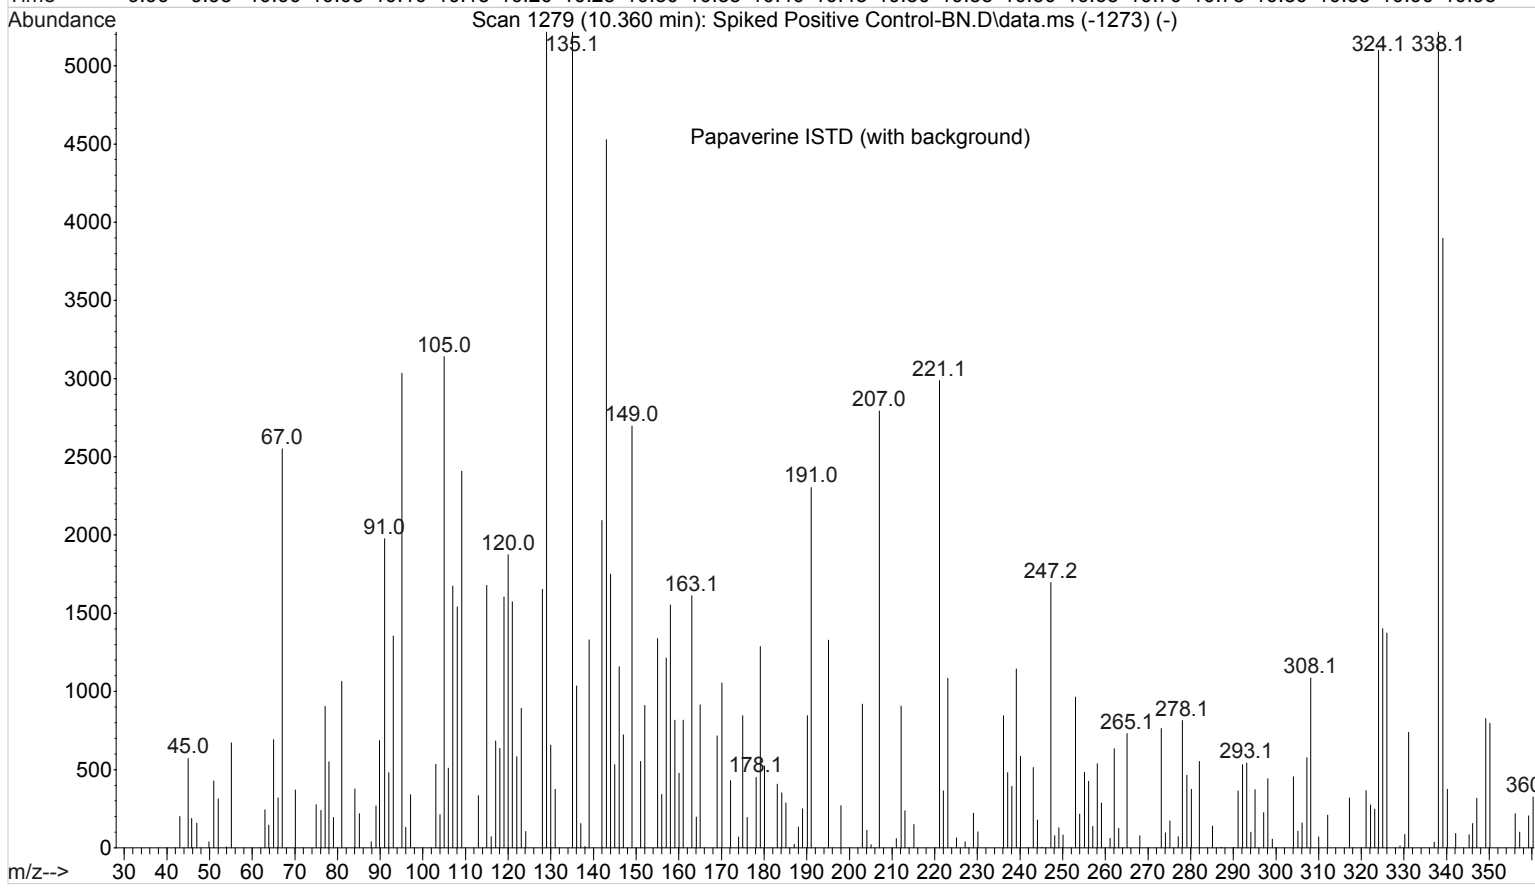
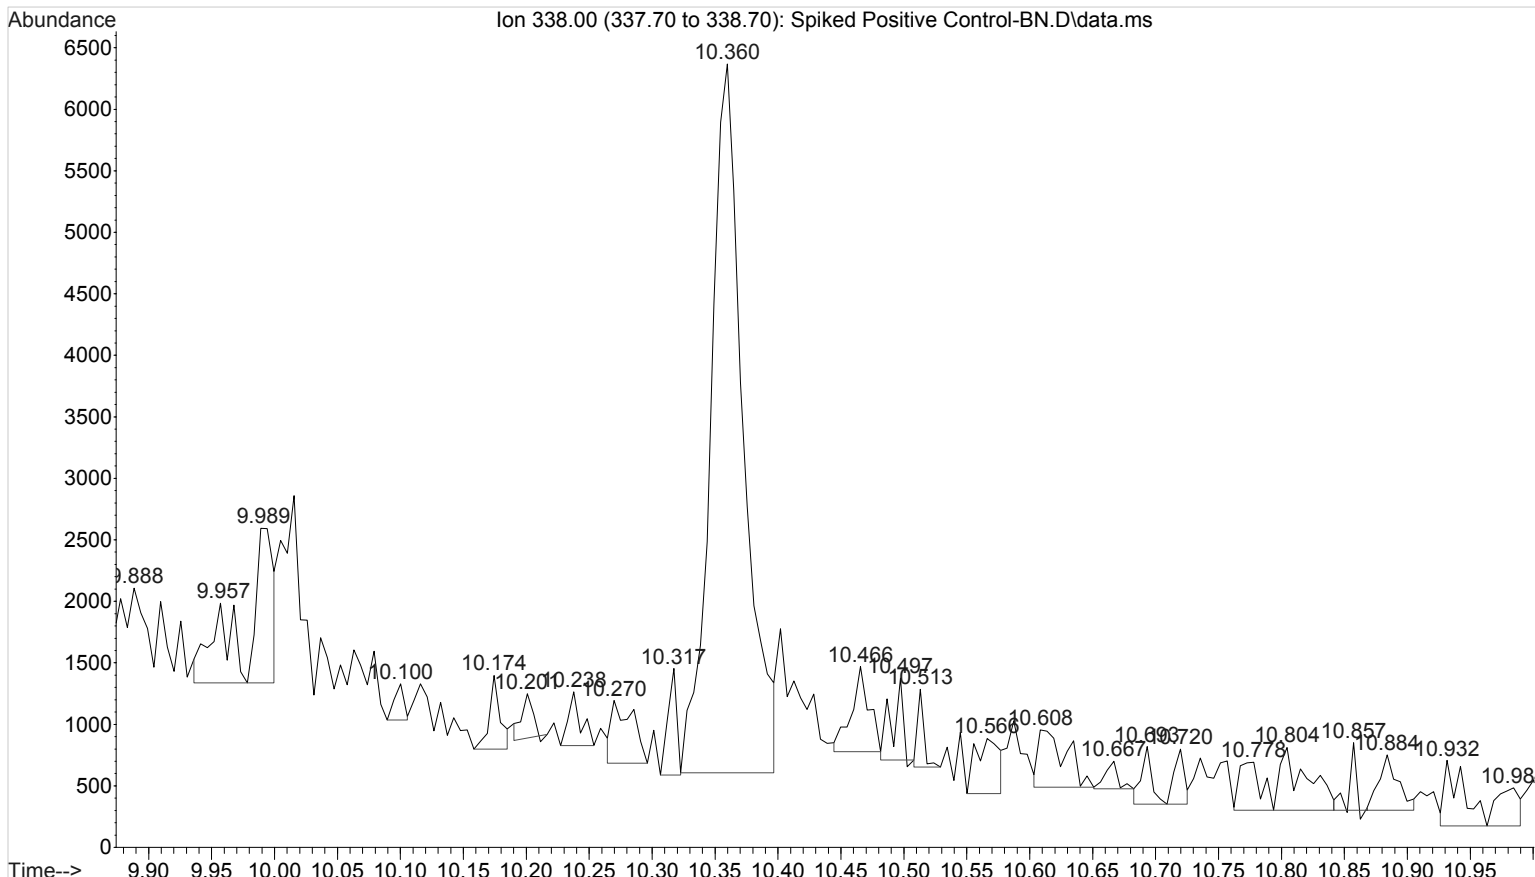


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Spiked Positive Control-BN.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 13:34 using AcqMethod BNSB120510.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

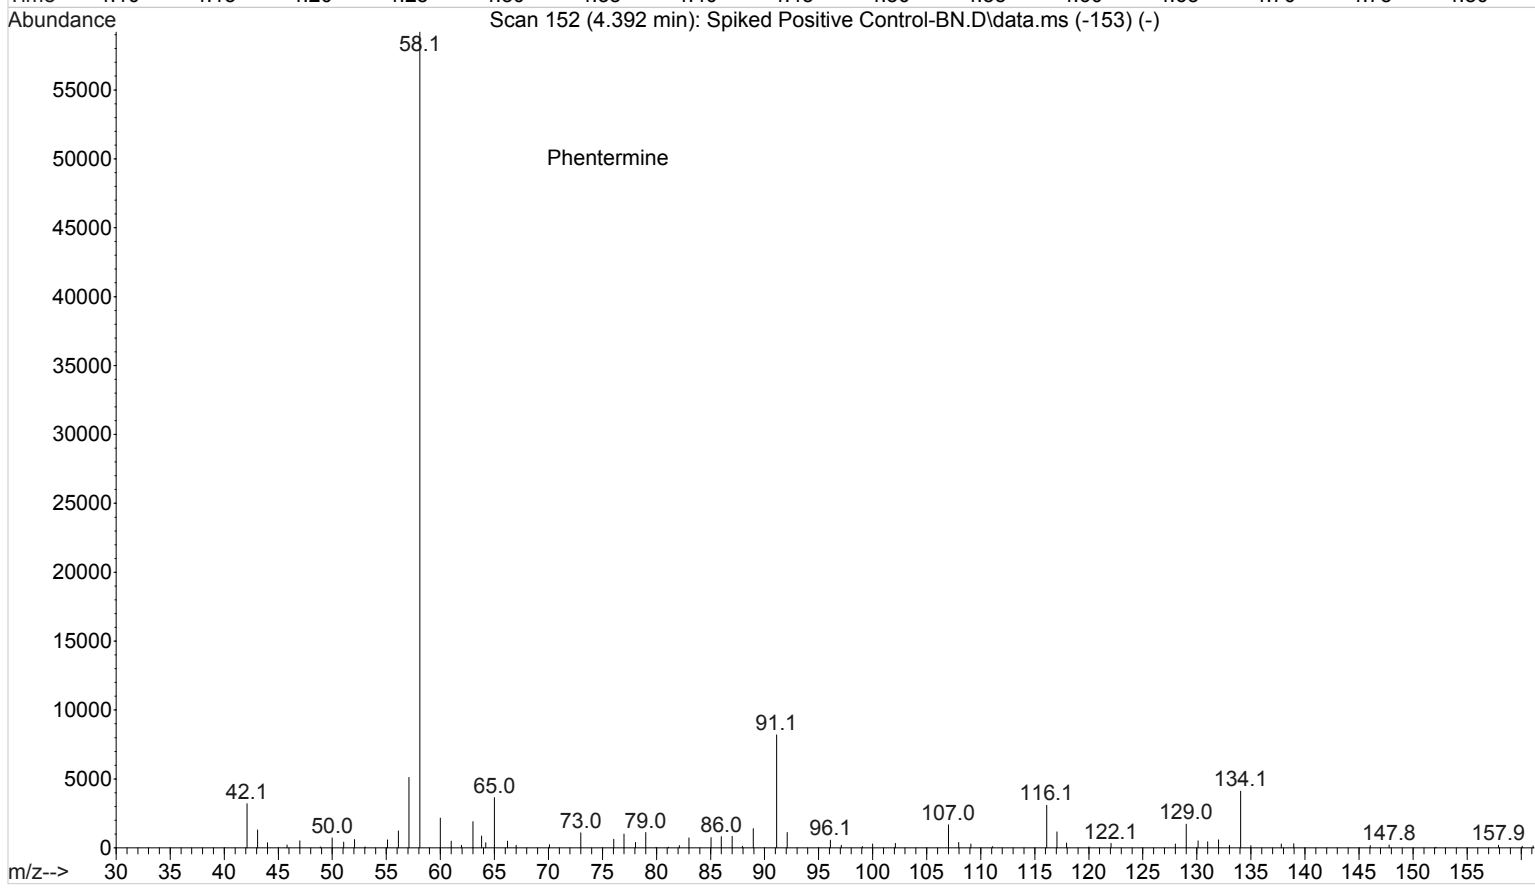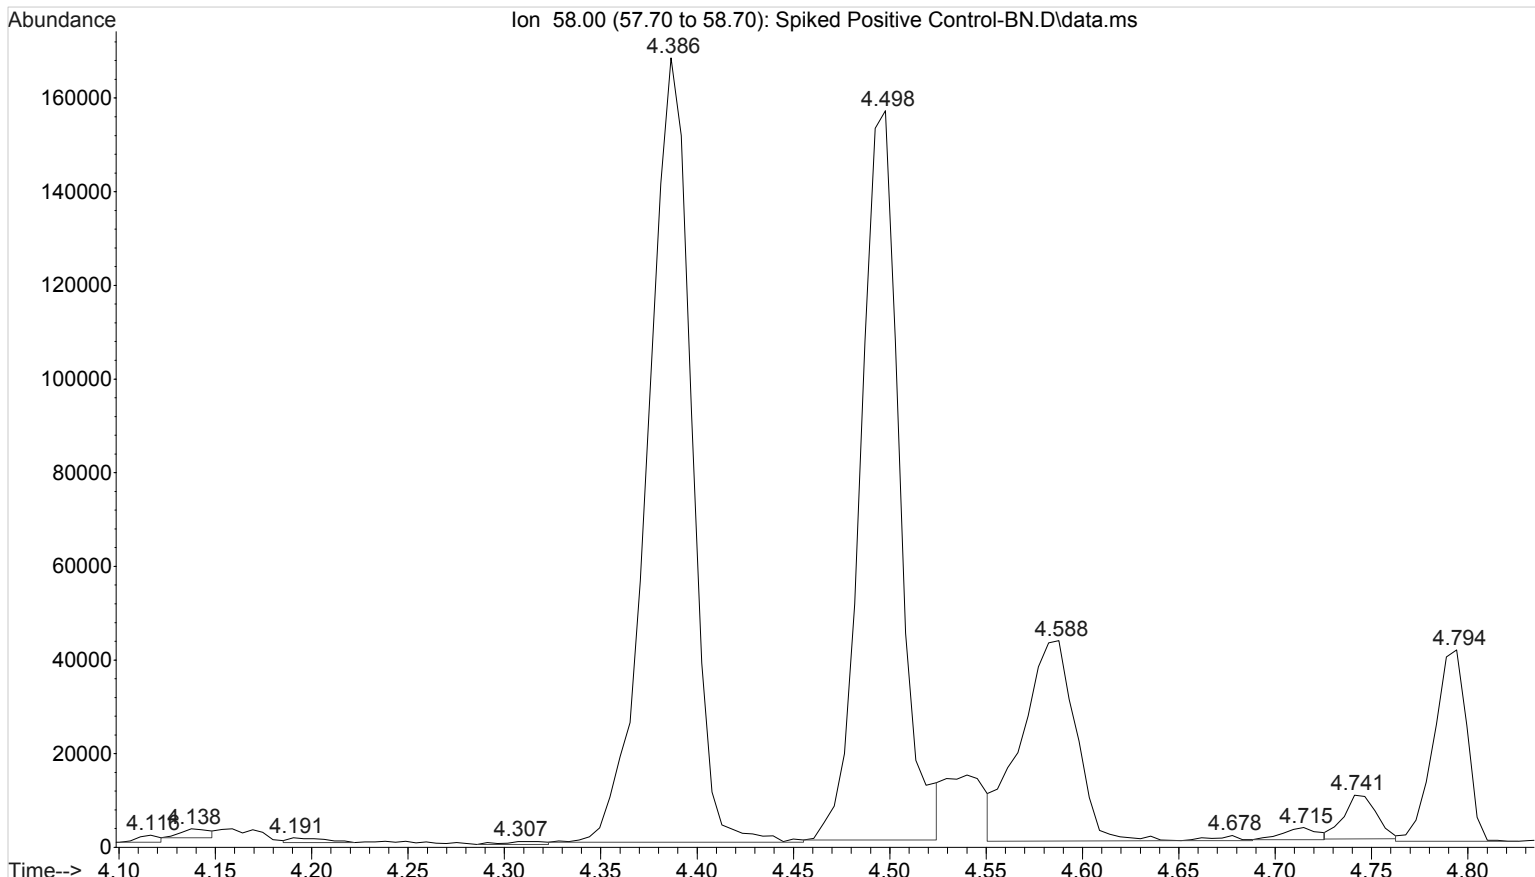



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Spiked Positive Control-BN.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 13:34 using AcqMethod BNSB120510.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

6

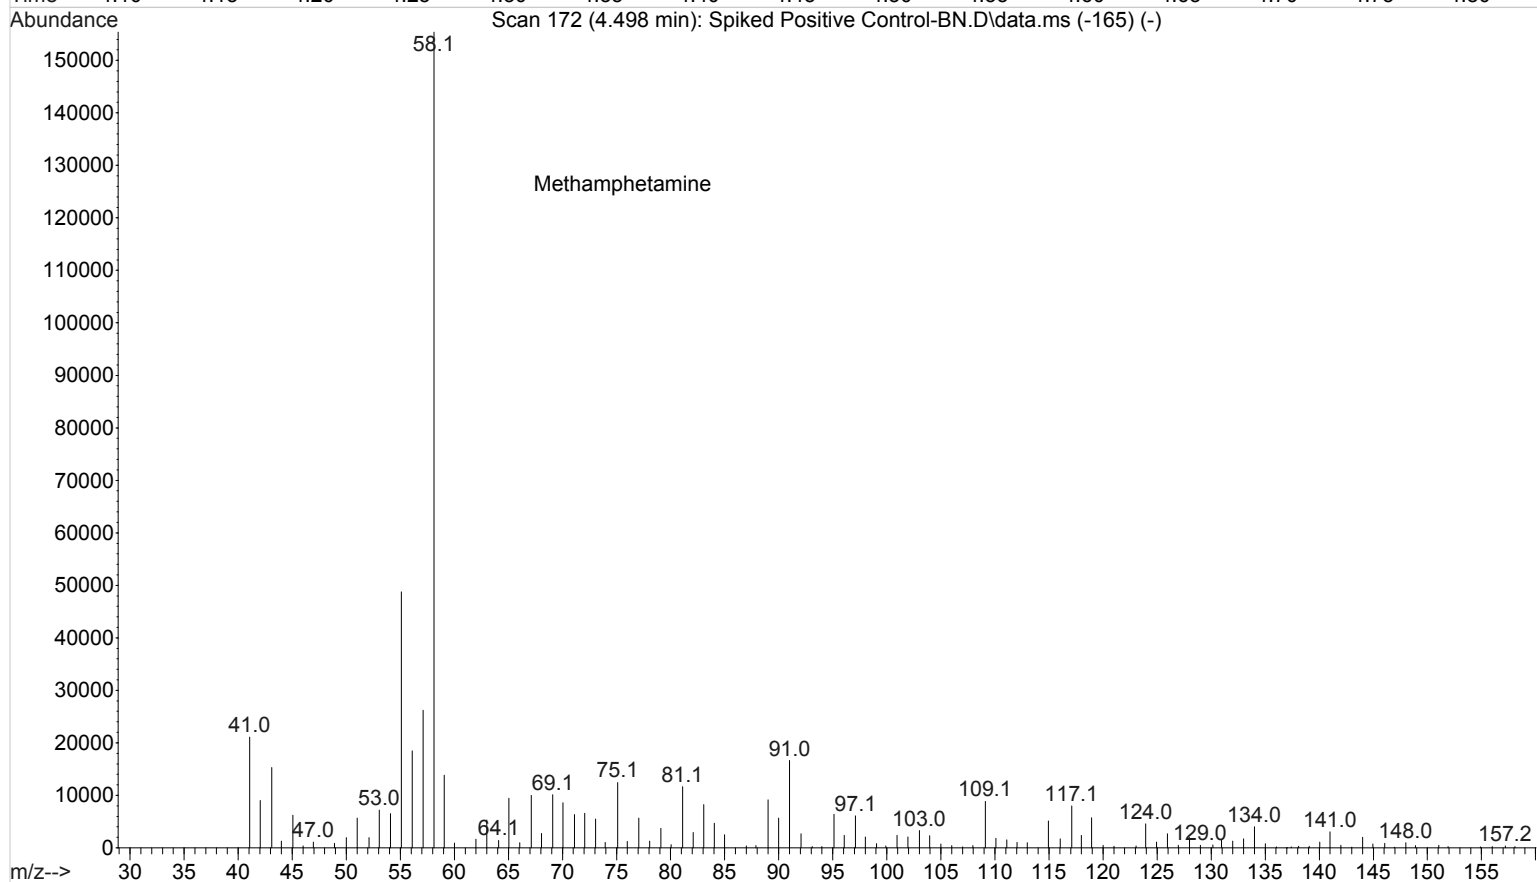
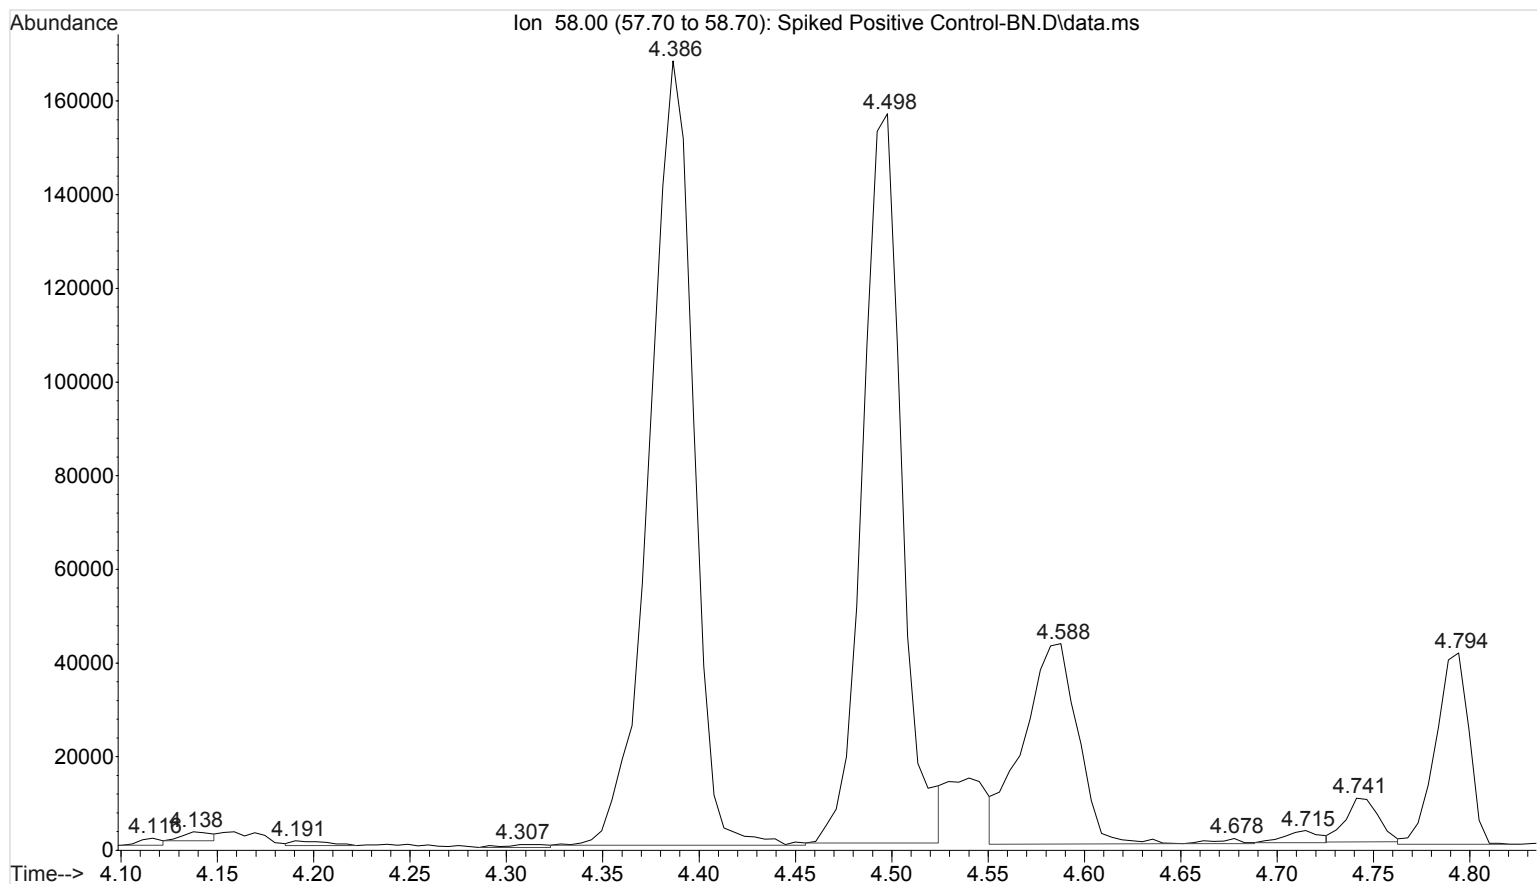






File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Spiked Positive Control-BN.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 13:34 using AcqMethod BNSB120510.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

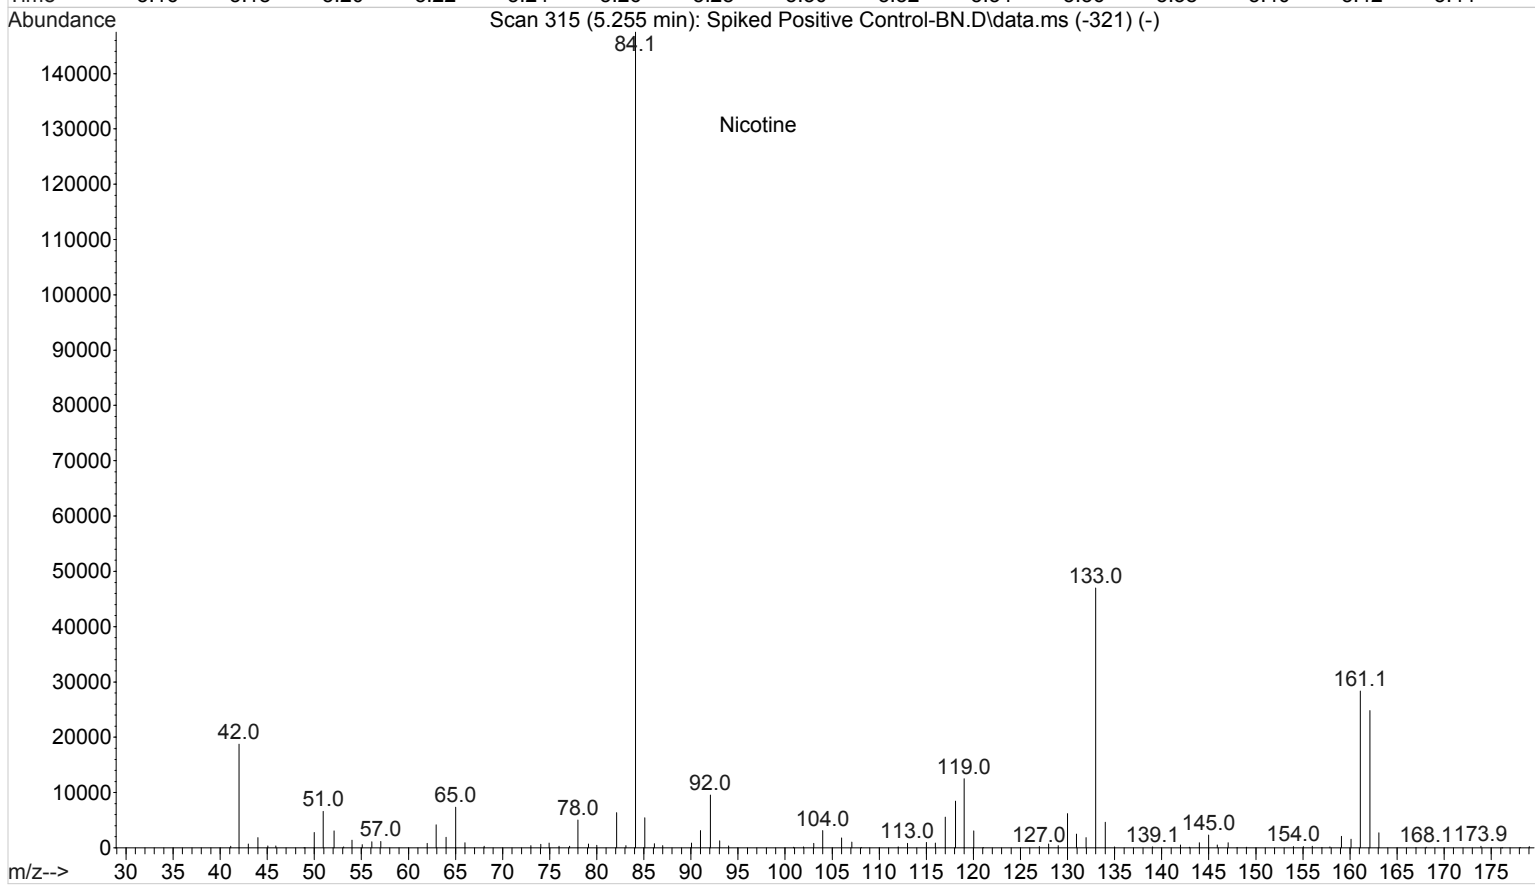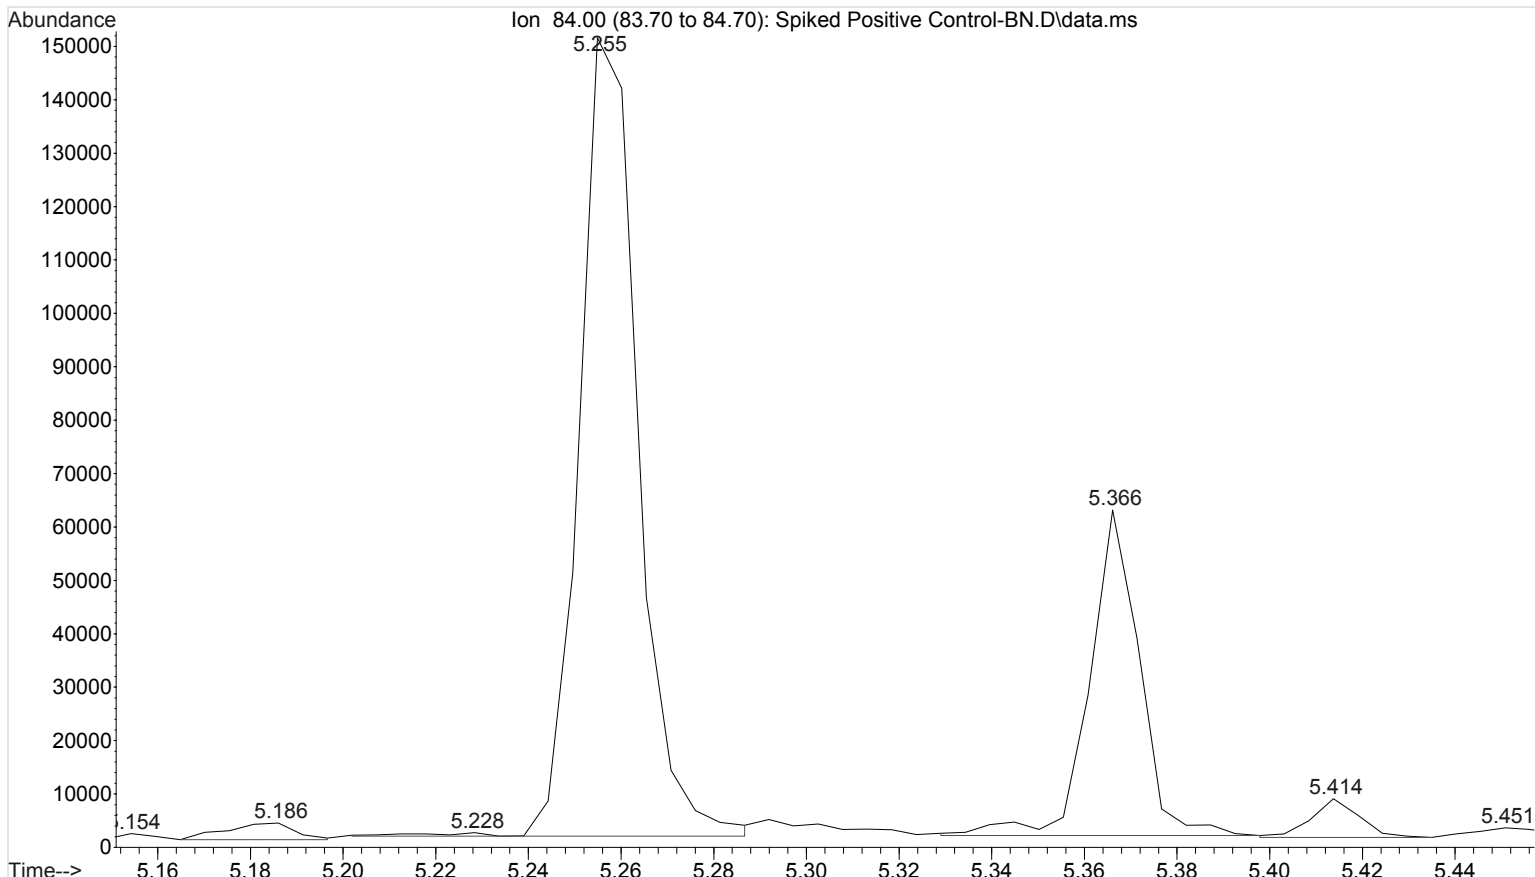



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Spiked Positive Control-BN.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 13:34 using AcqMethod BNSB120510.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

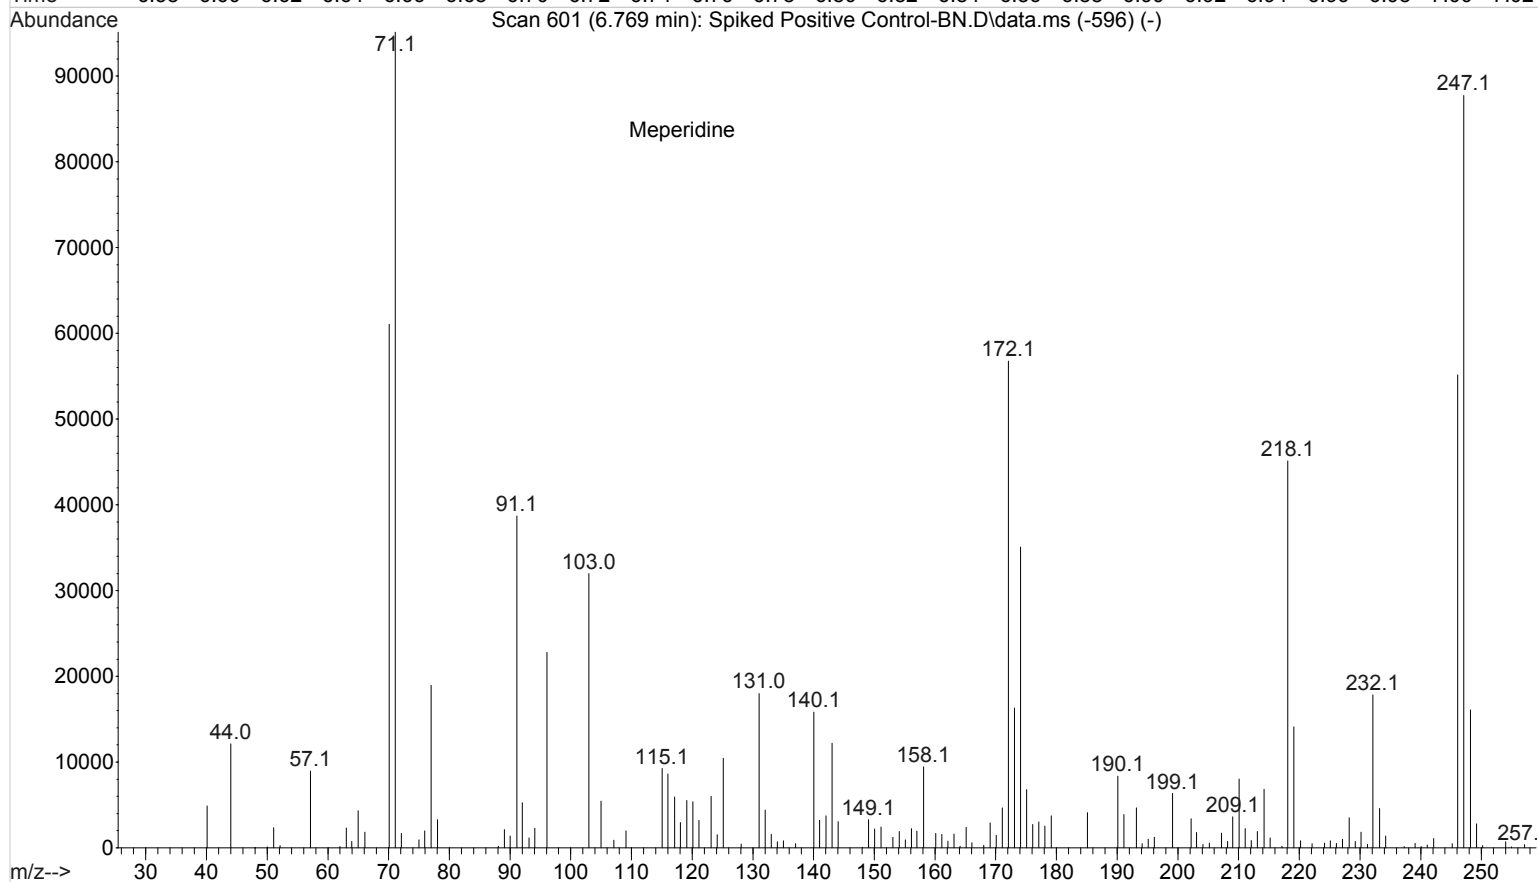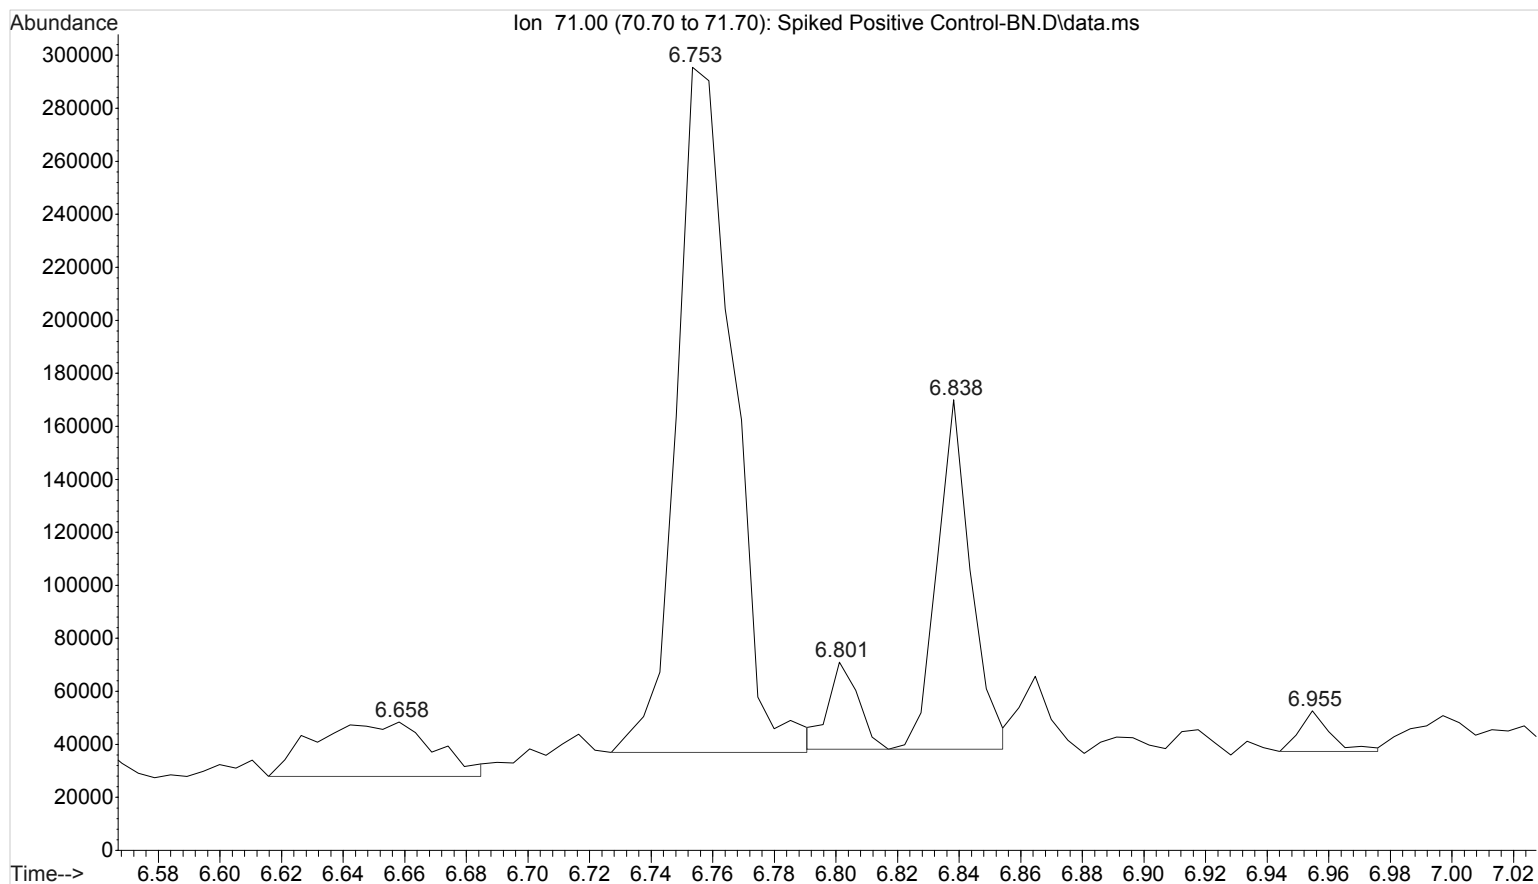



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Spiked Positive Control-BN.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 13:34 using AcqMethod BNSB120510.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

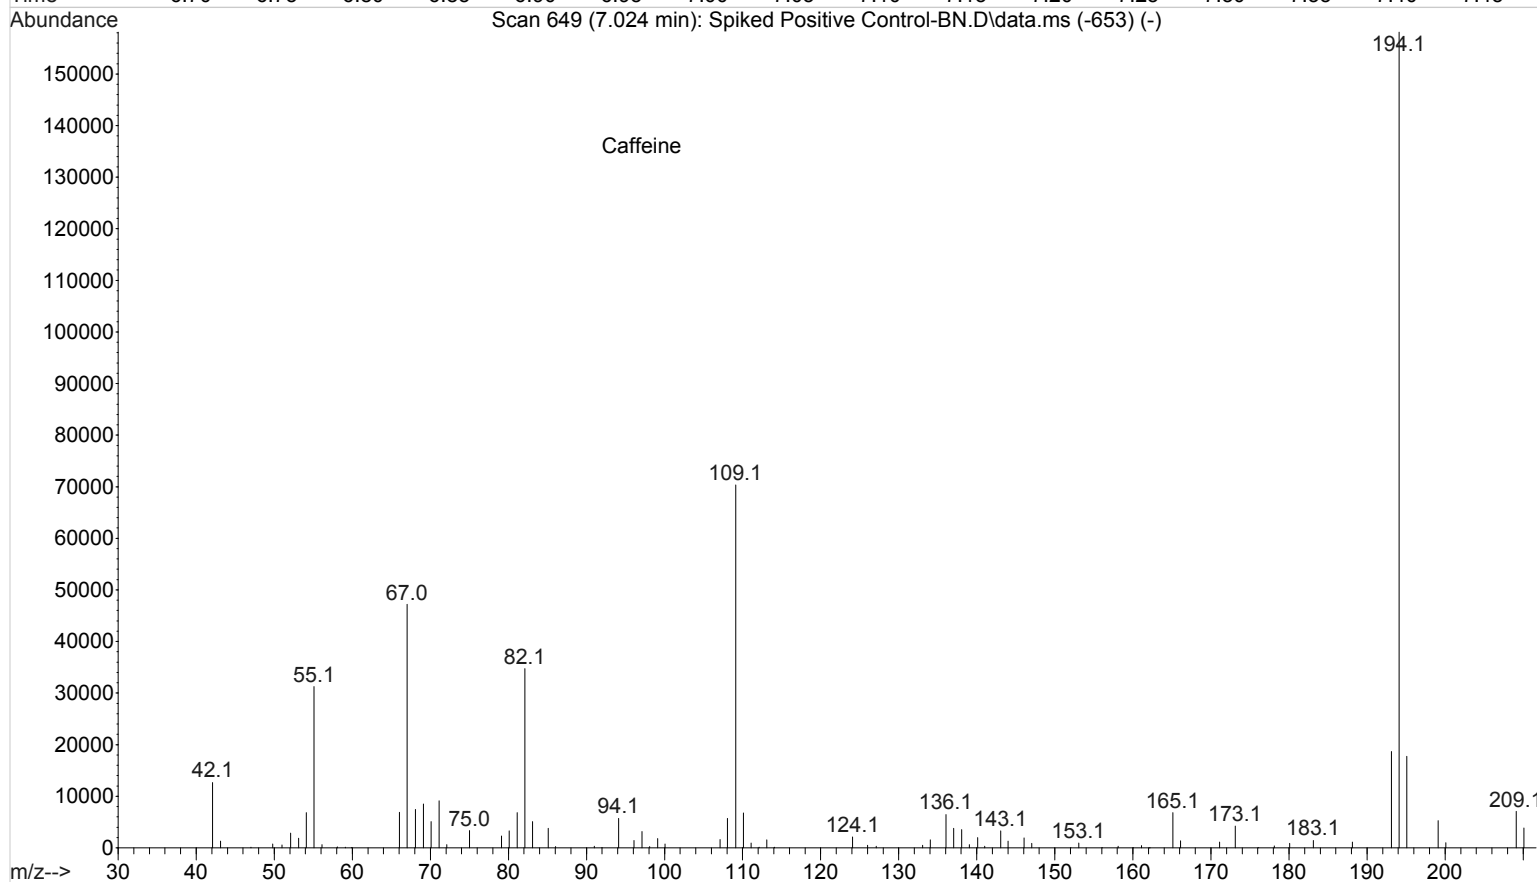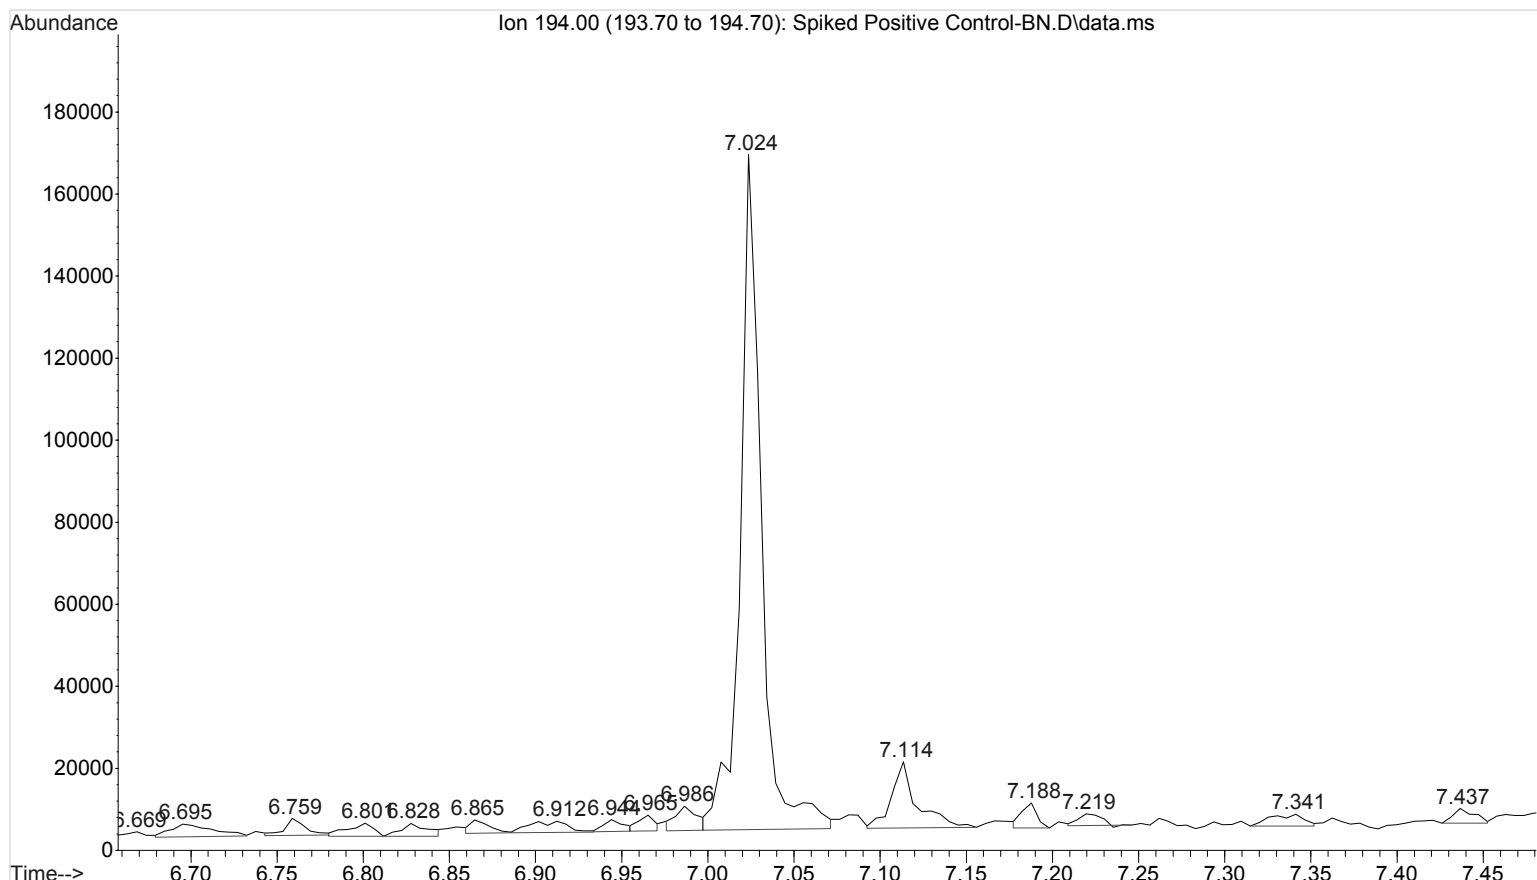



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Spiked Positive Control-BN.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 13:34 using AcqMethod BNSB120510.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

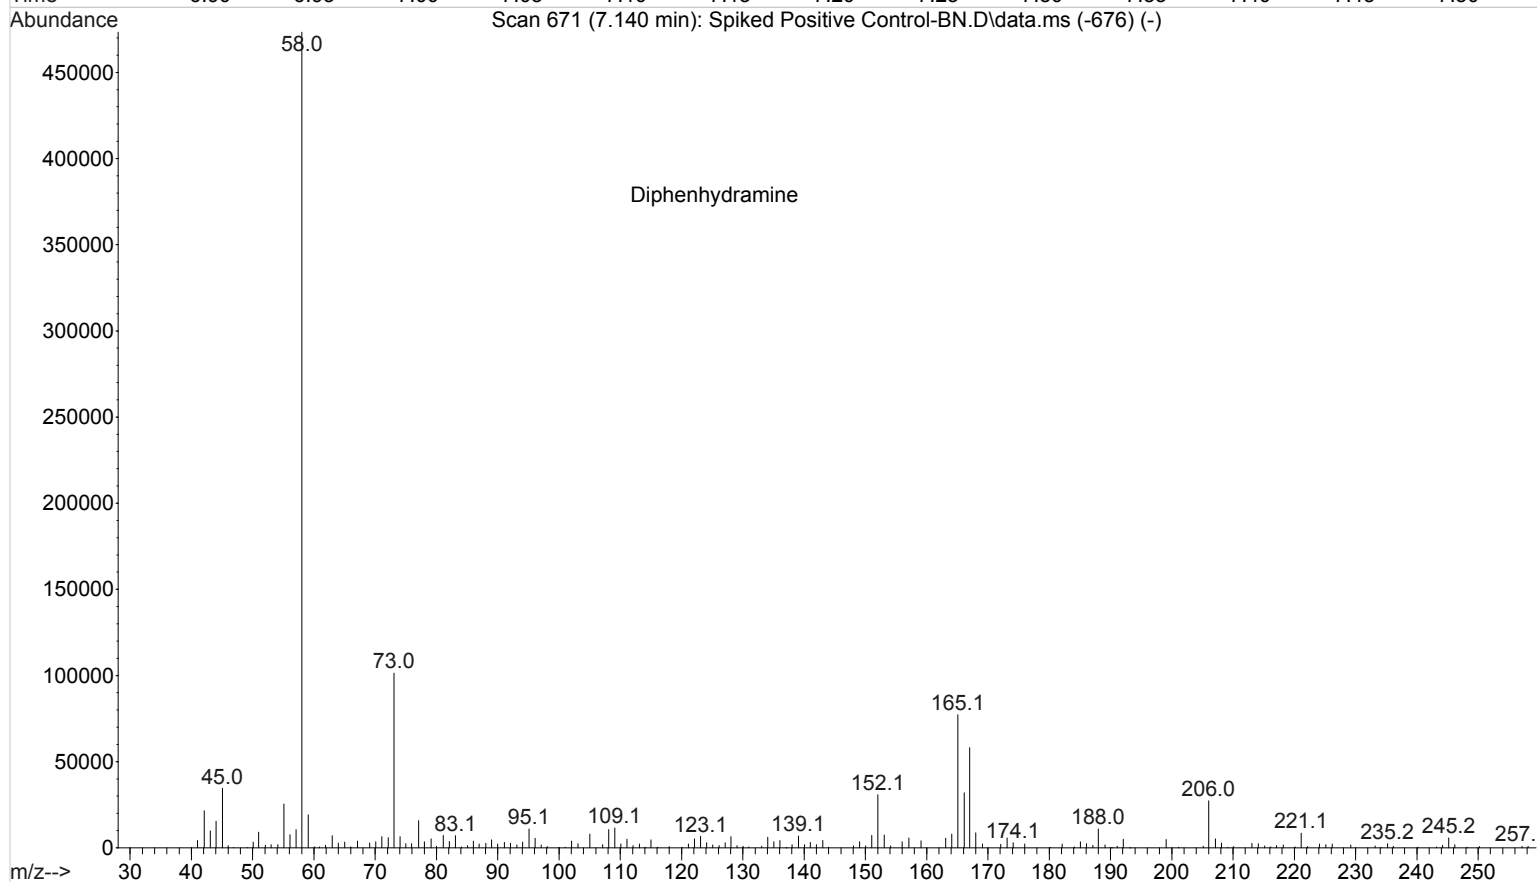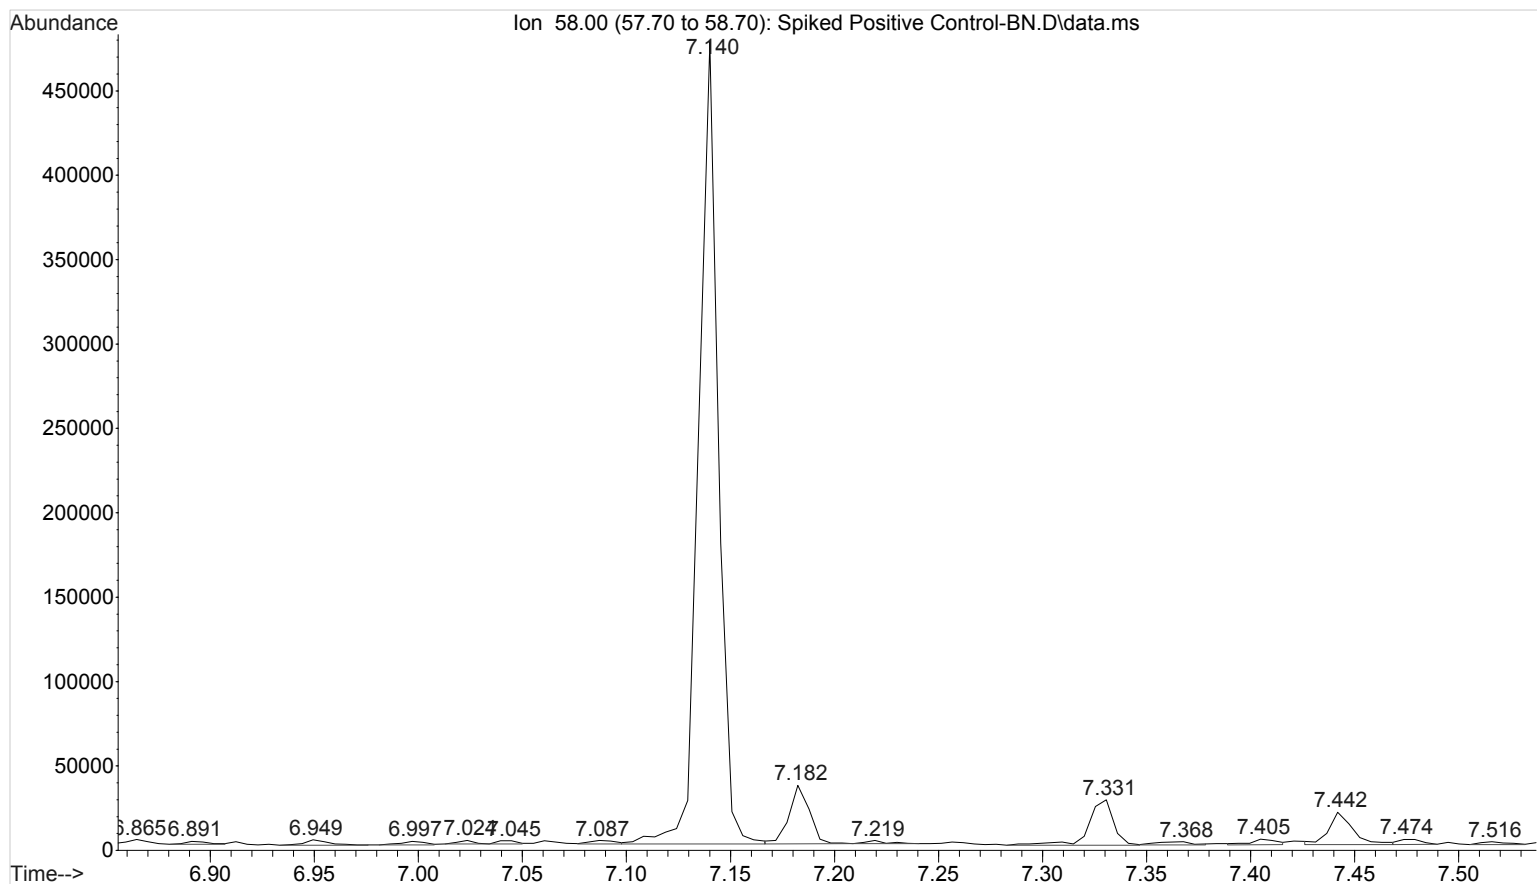

File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Spiked Positive Control-BN.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 13:34 using AcqMethod BNSB120510.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

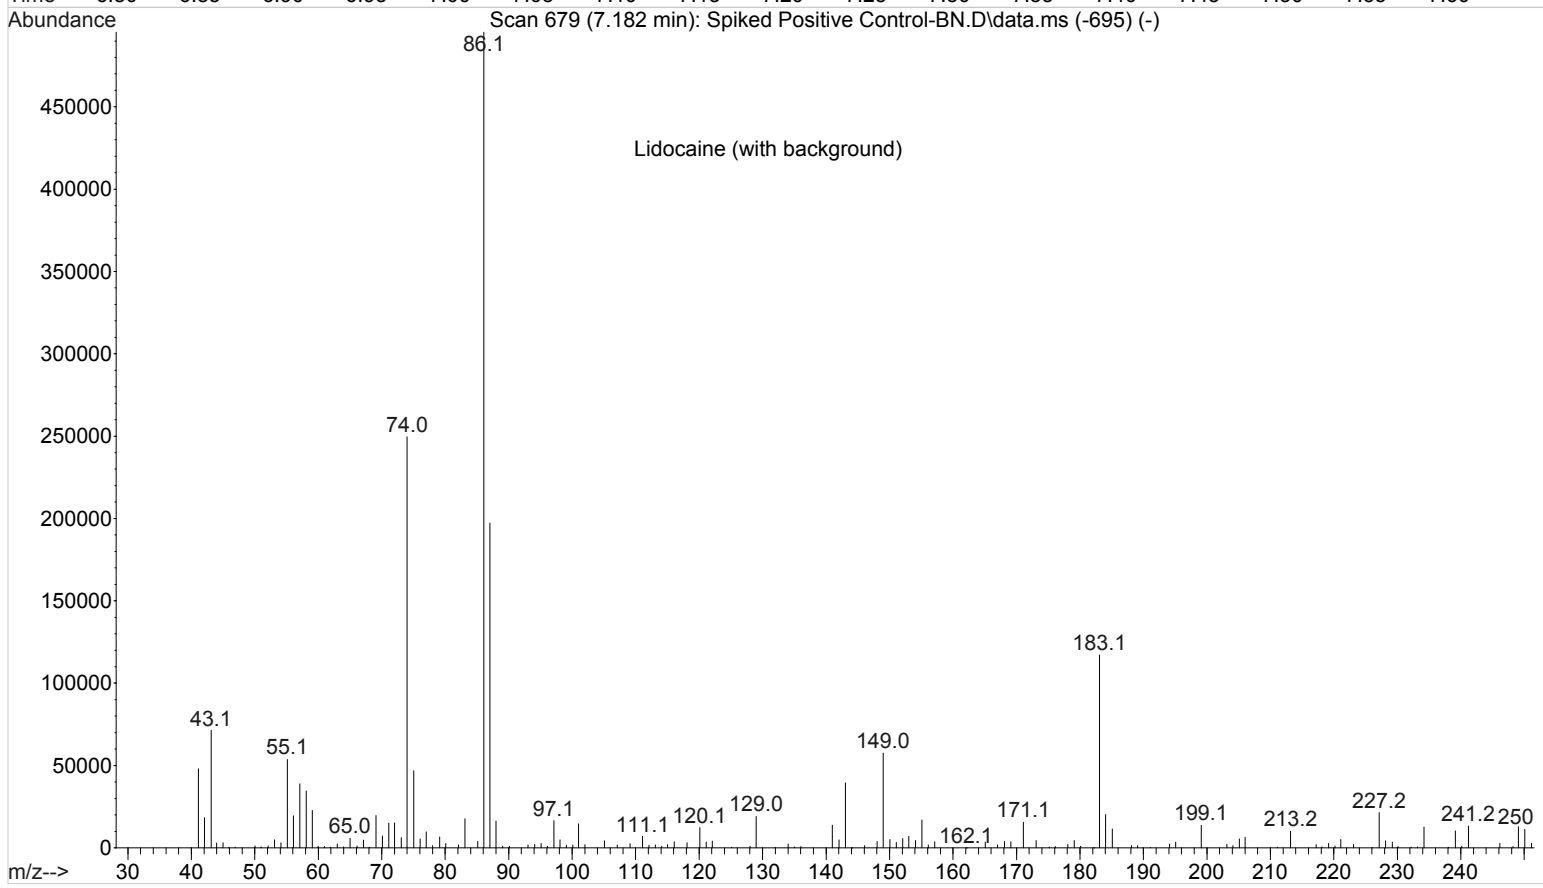
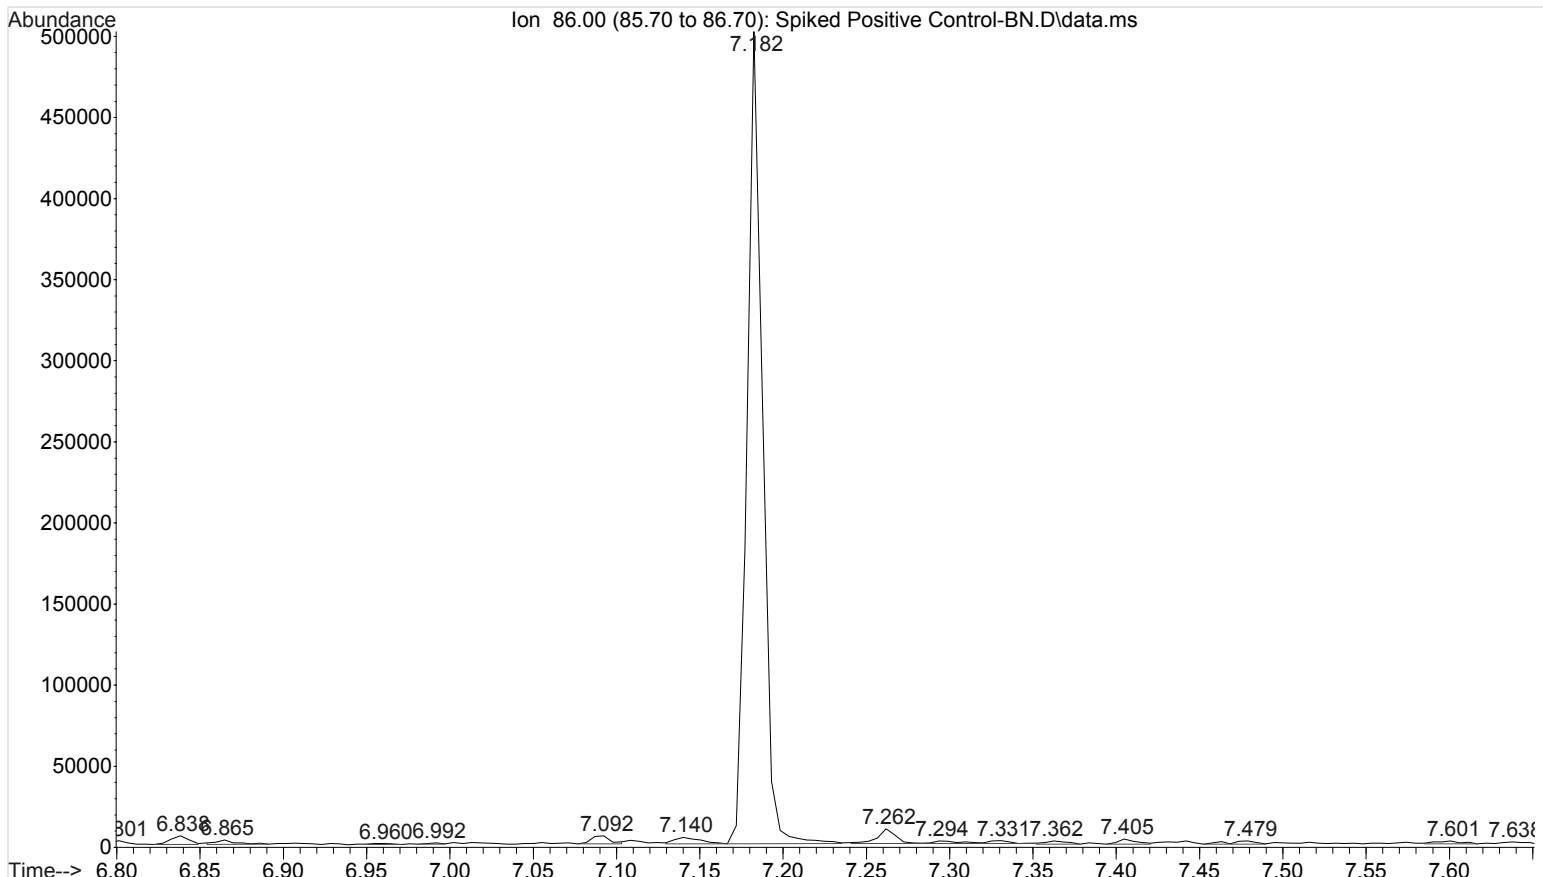


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Spiked Positive Control-BN.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 13:34 using AcqMethod BNSB120510.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

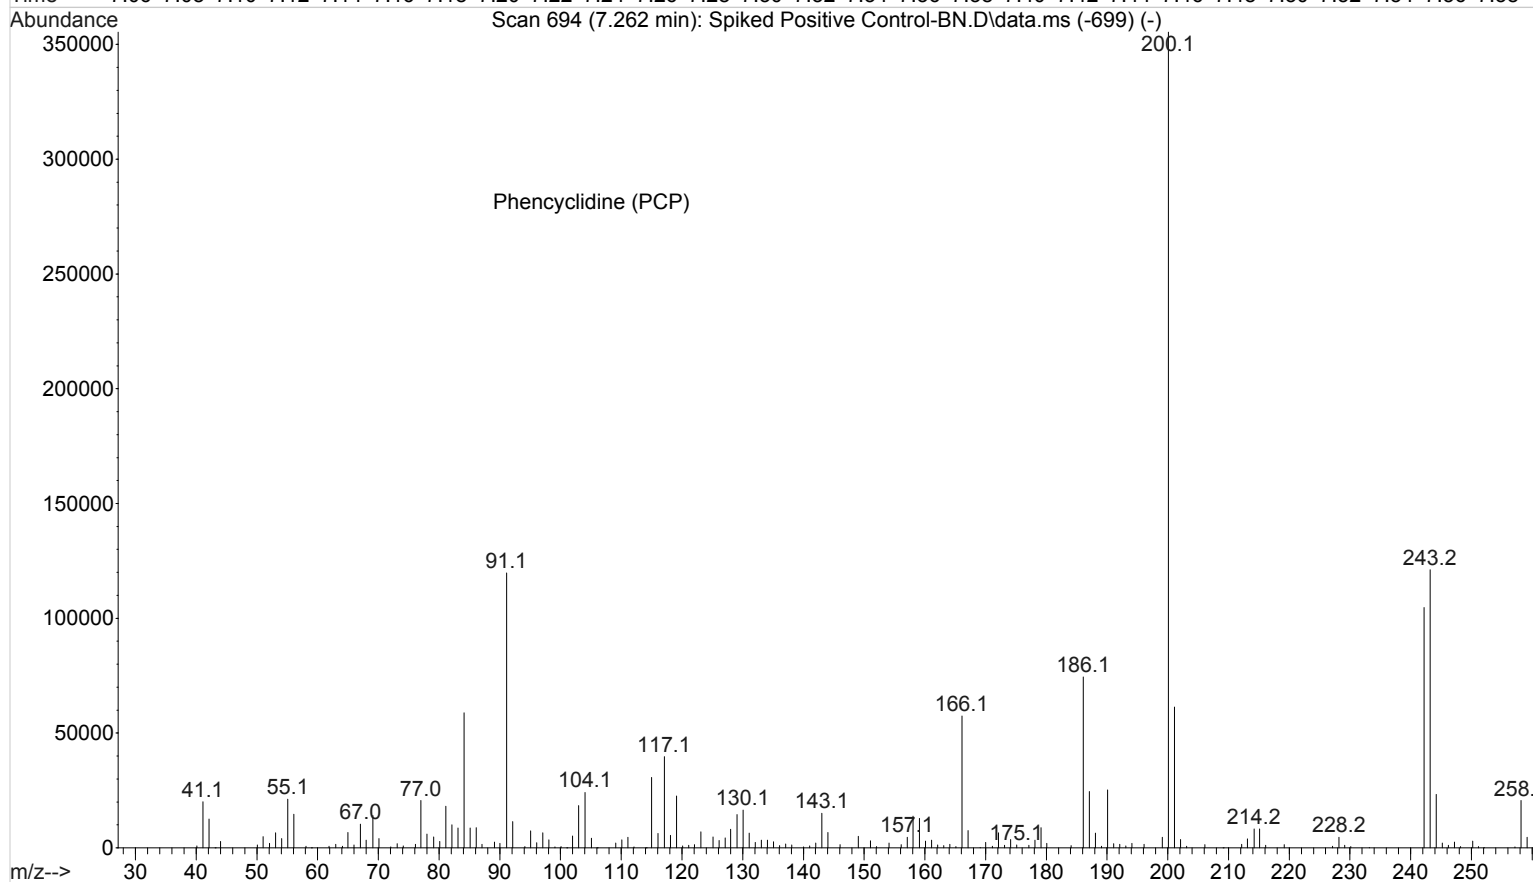
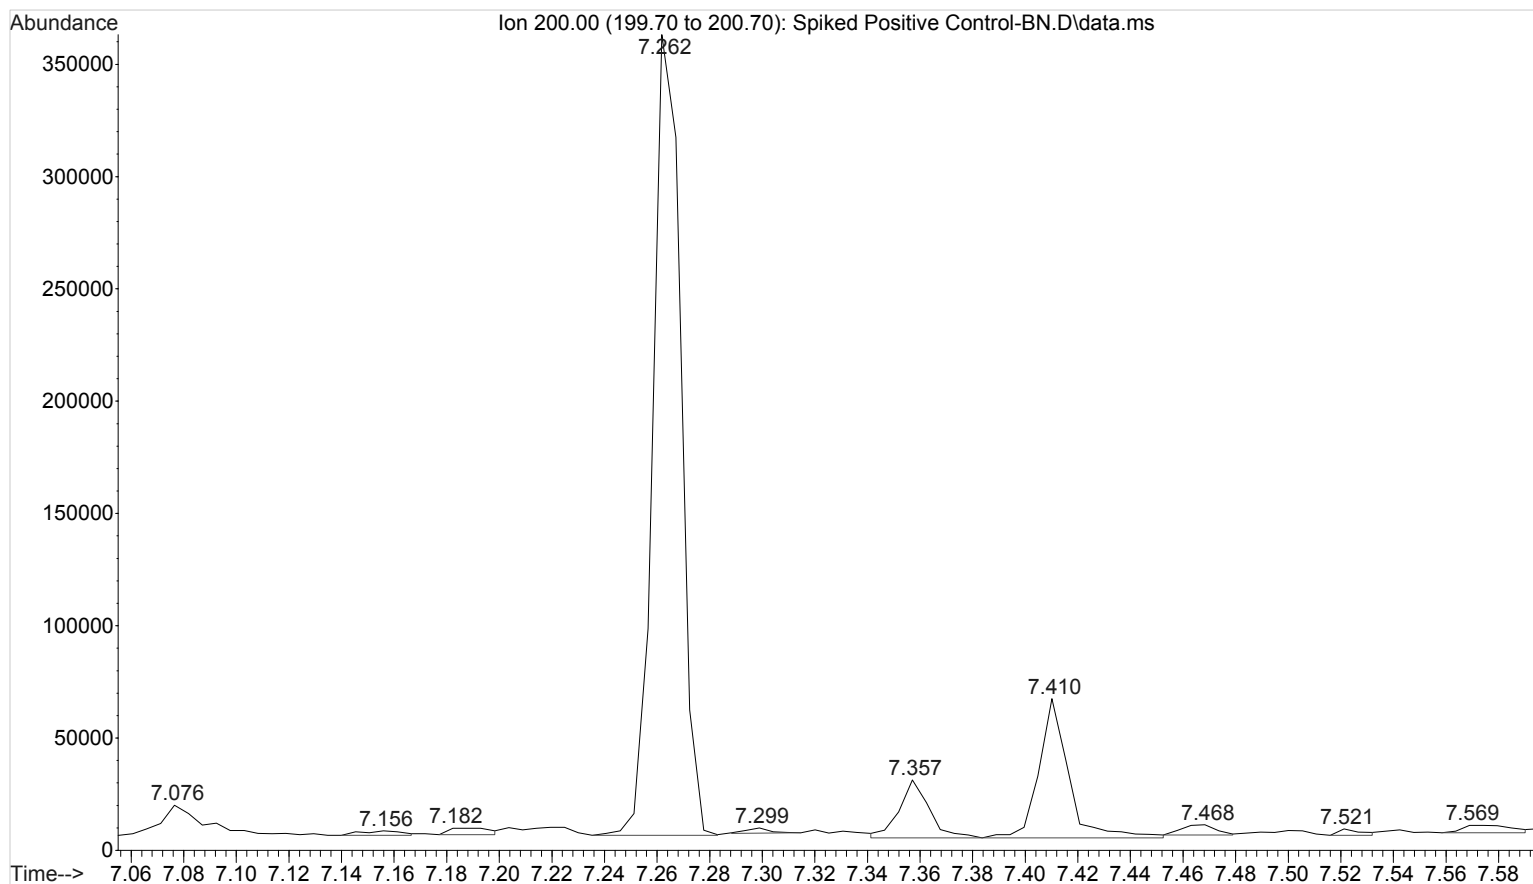


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Spiked Positive Control-BN.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 13:34 using AcqMethod BNSB120510.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

5

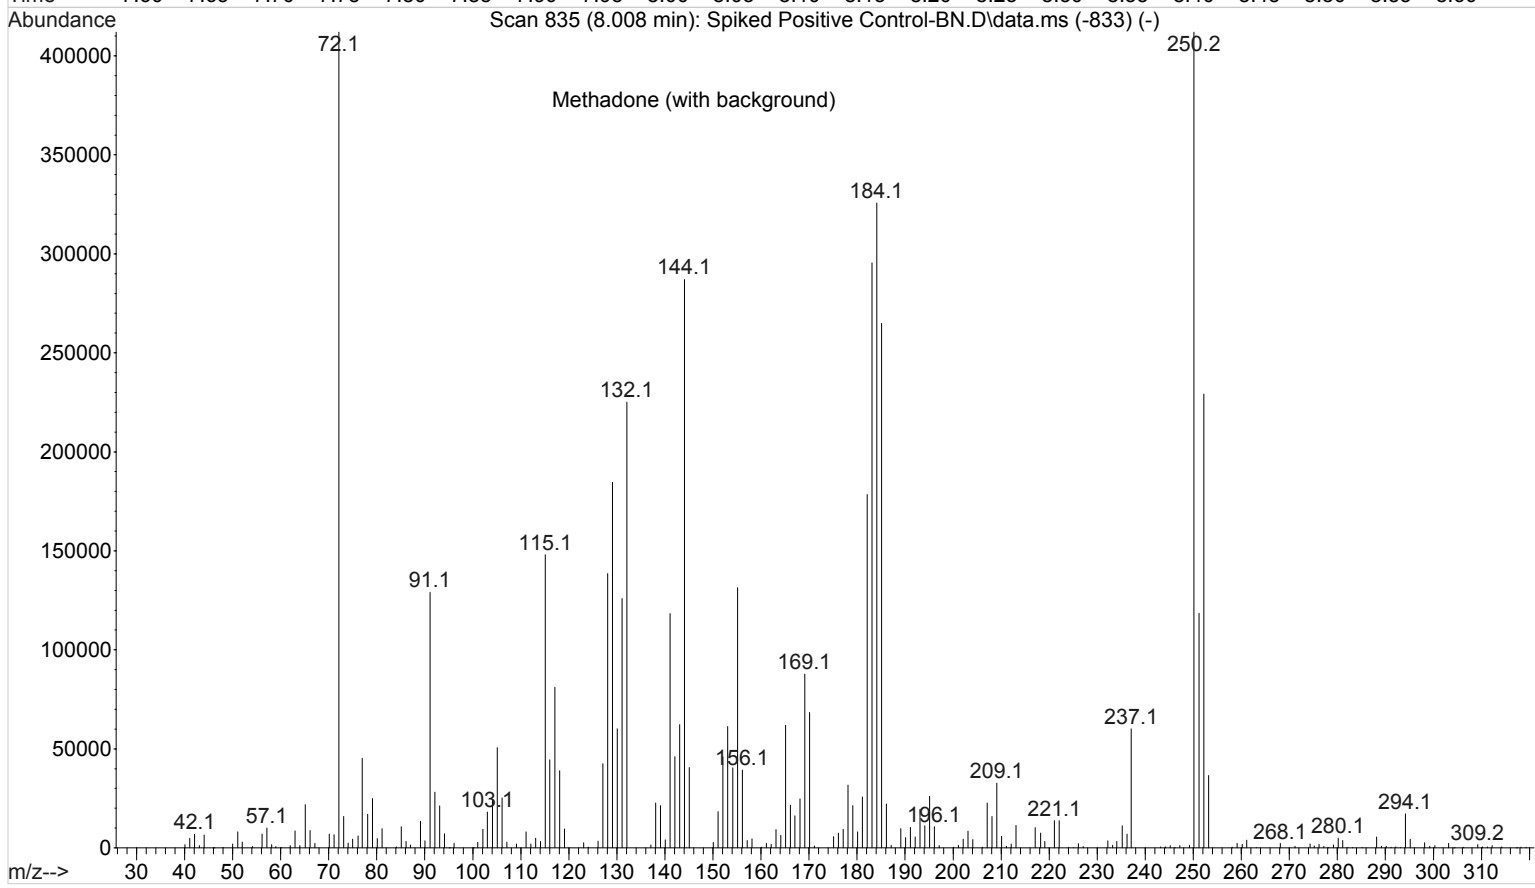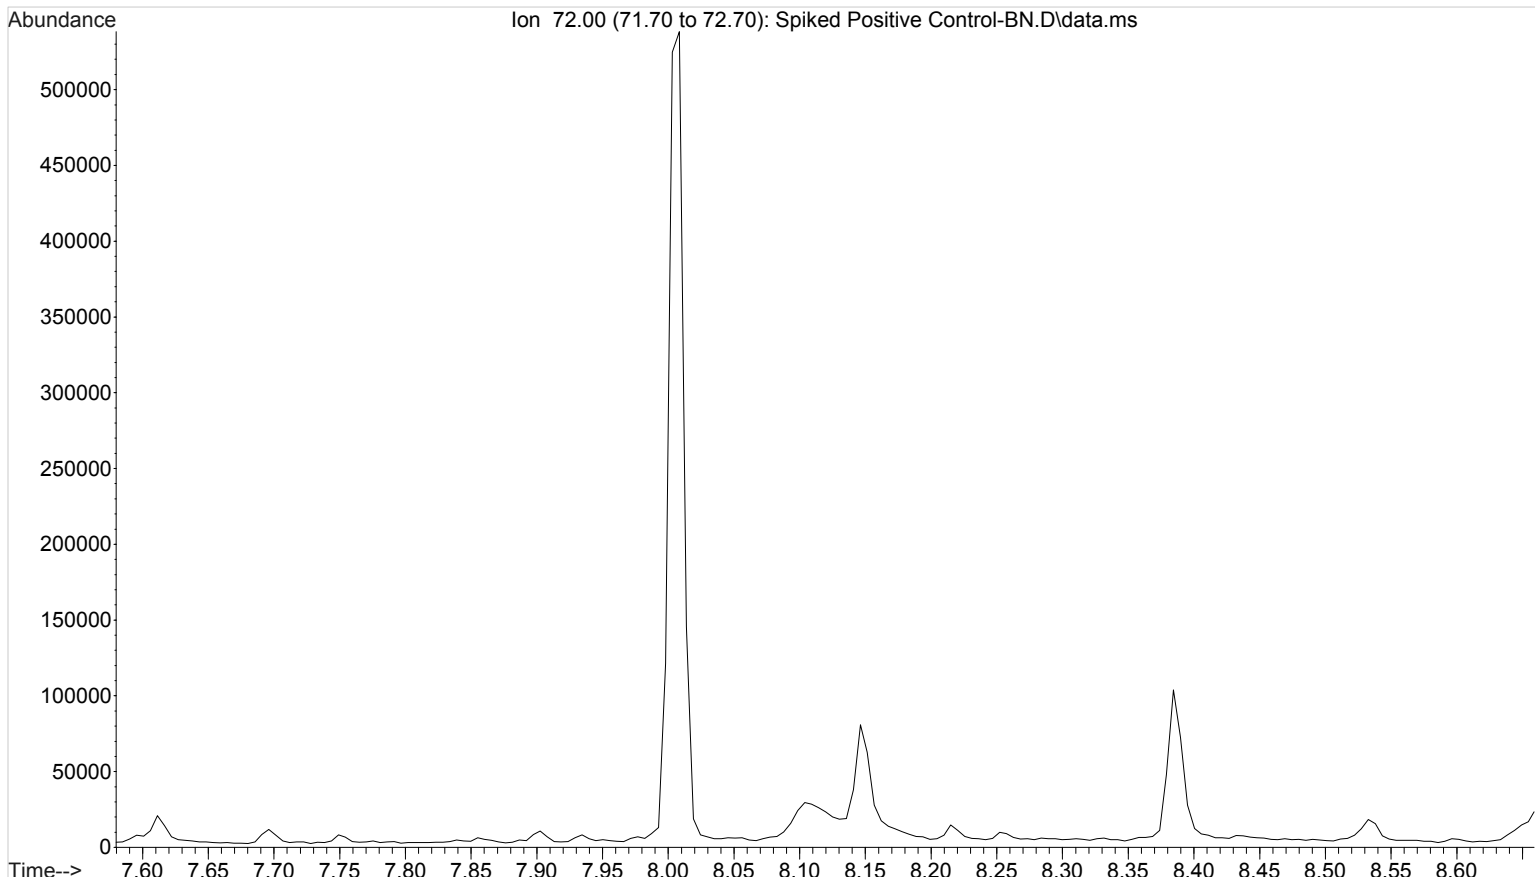



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Spiked Positive Control-BN.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 13:34 using AcqMethod BNSB120510.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

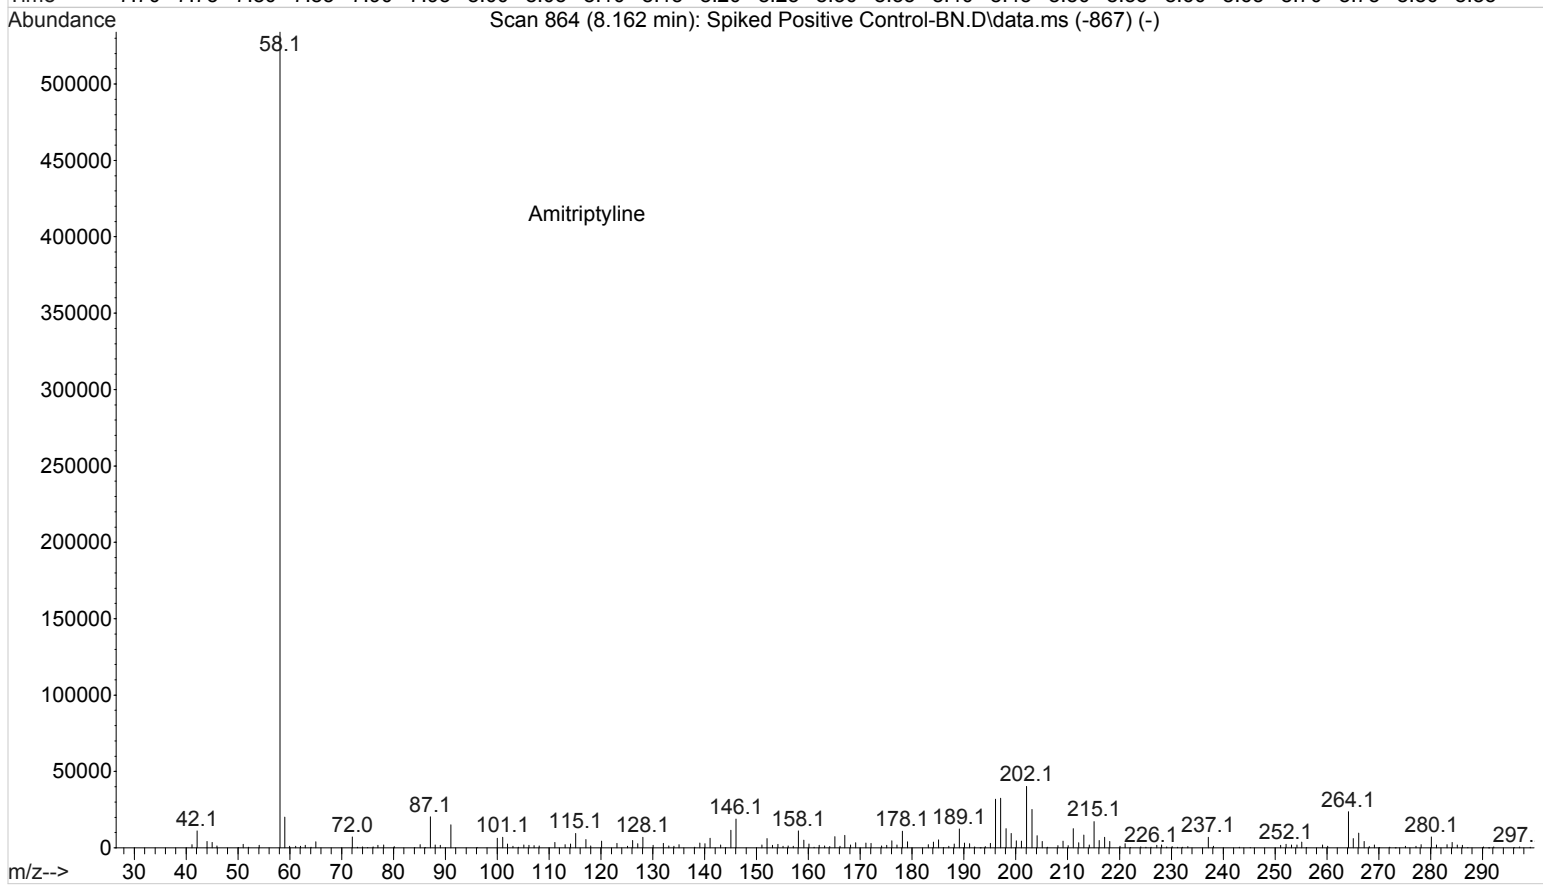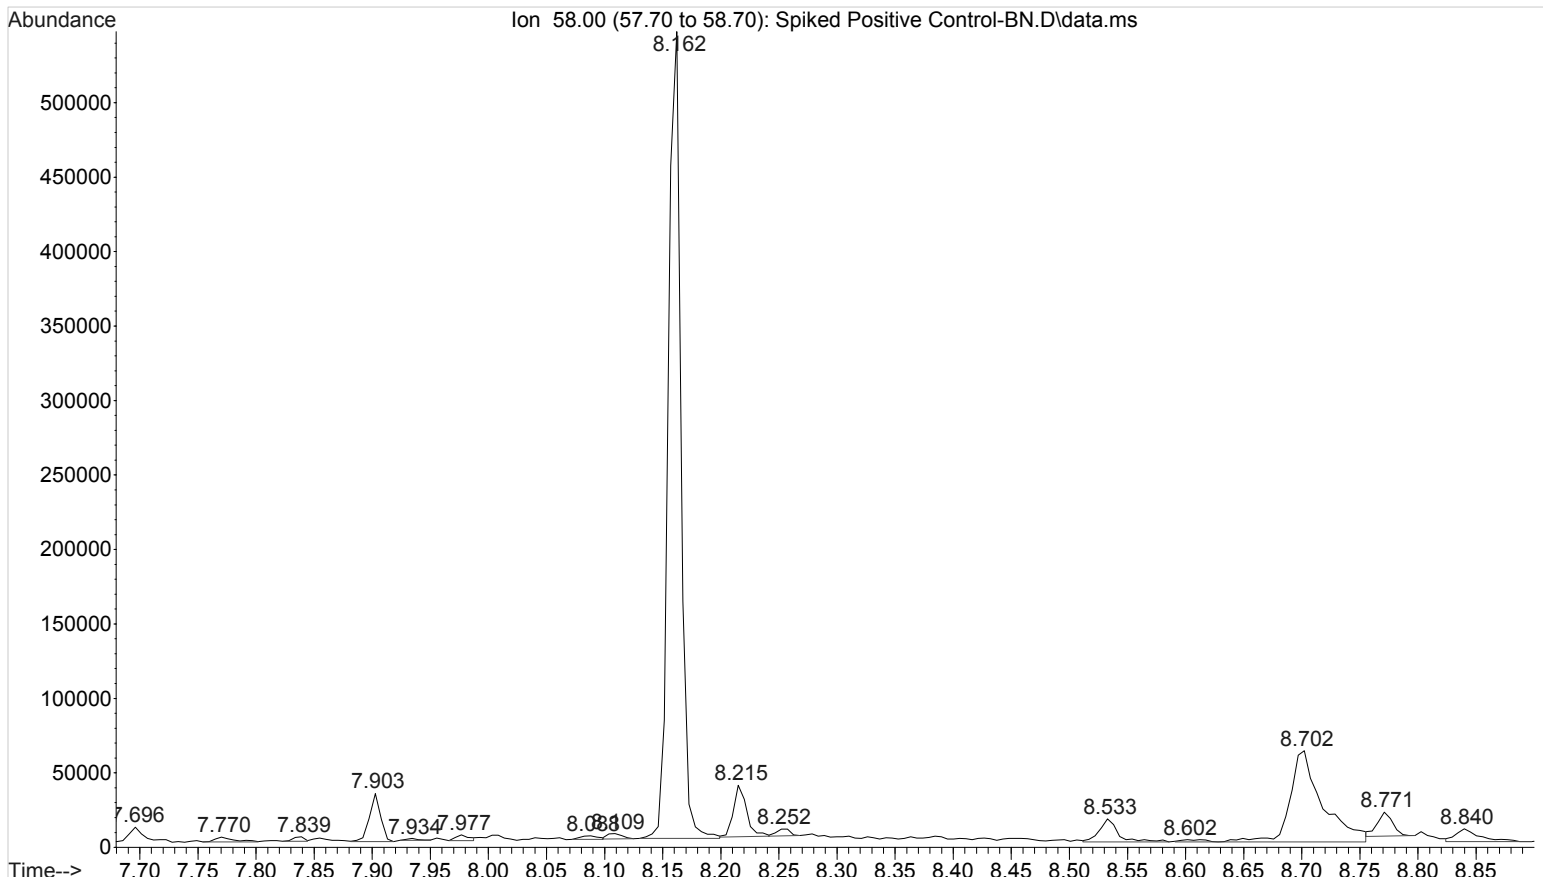





File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Spiked Positive Control-BN.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 13:34 using AcqMethod BNSB120510.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215


99

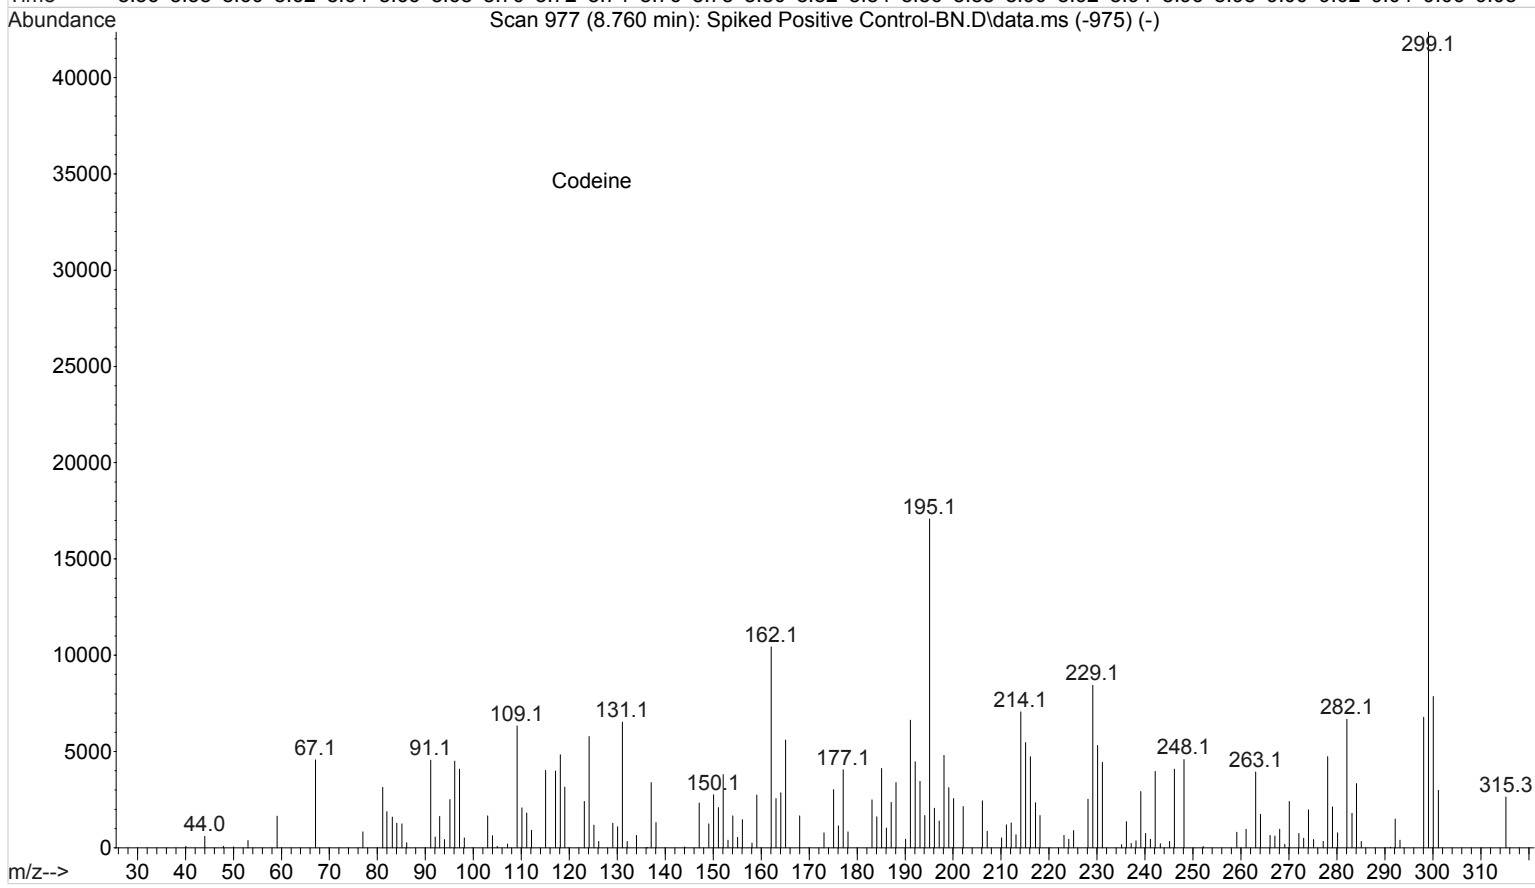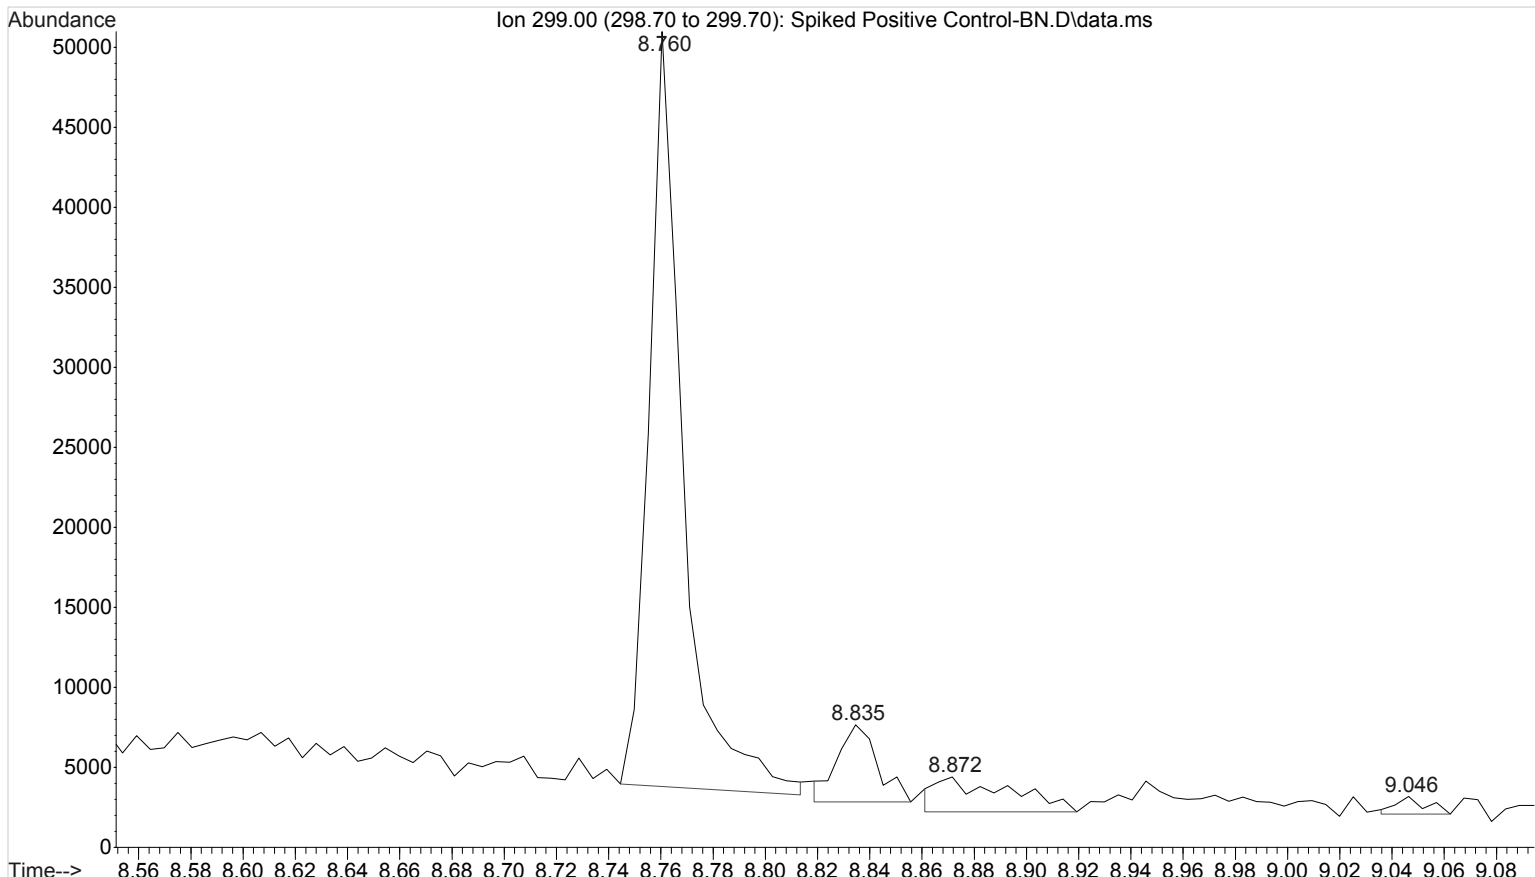

File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Spiked Positive Control-BN.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 13:34 using AcqMethod BNSB120510.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

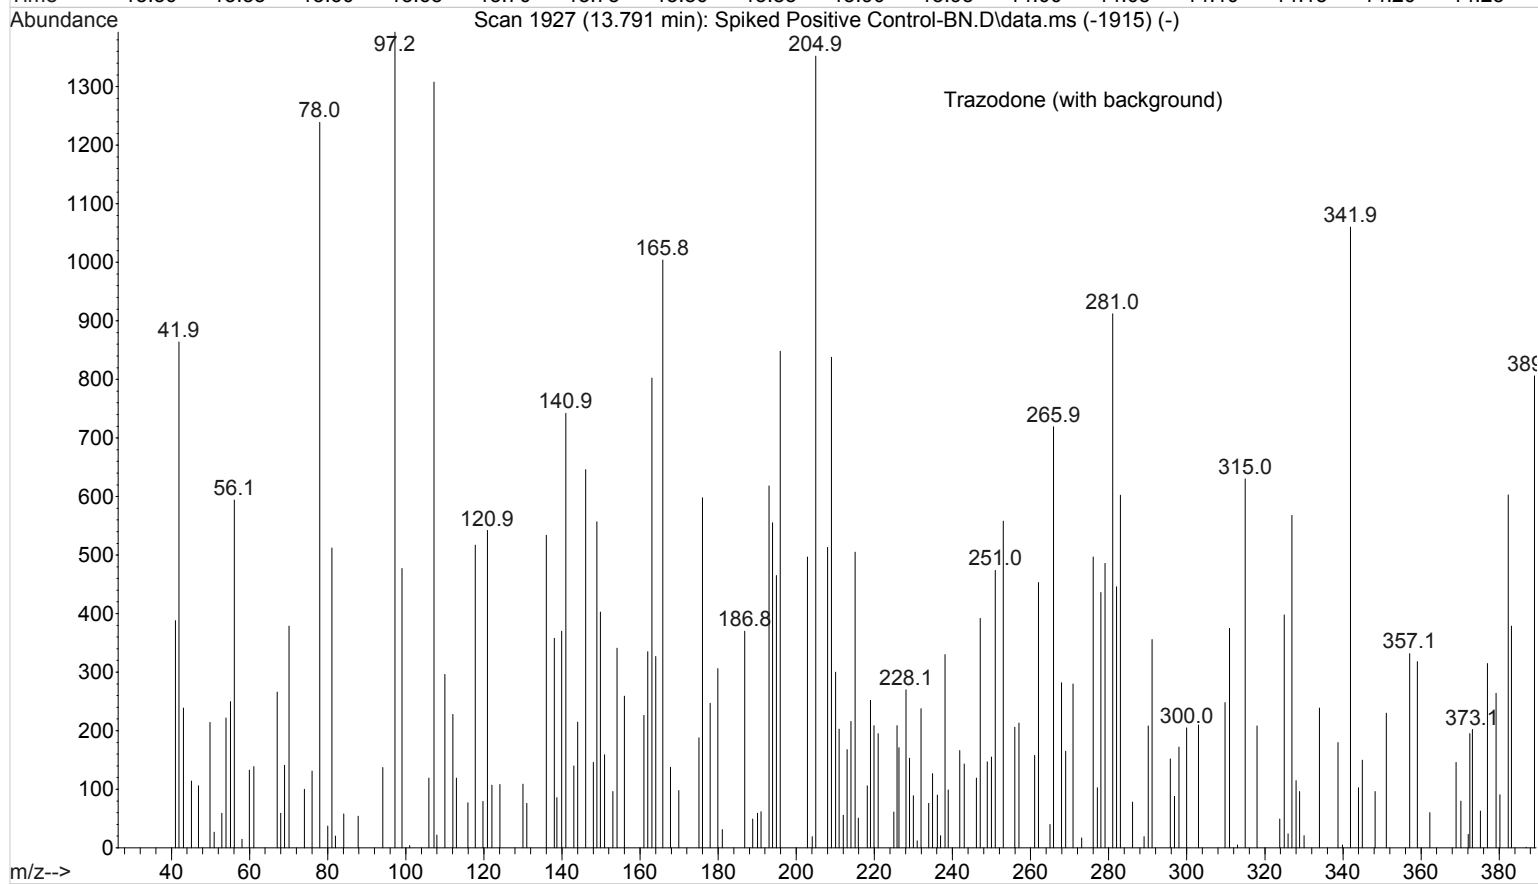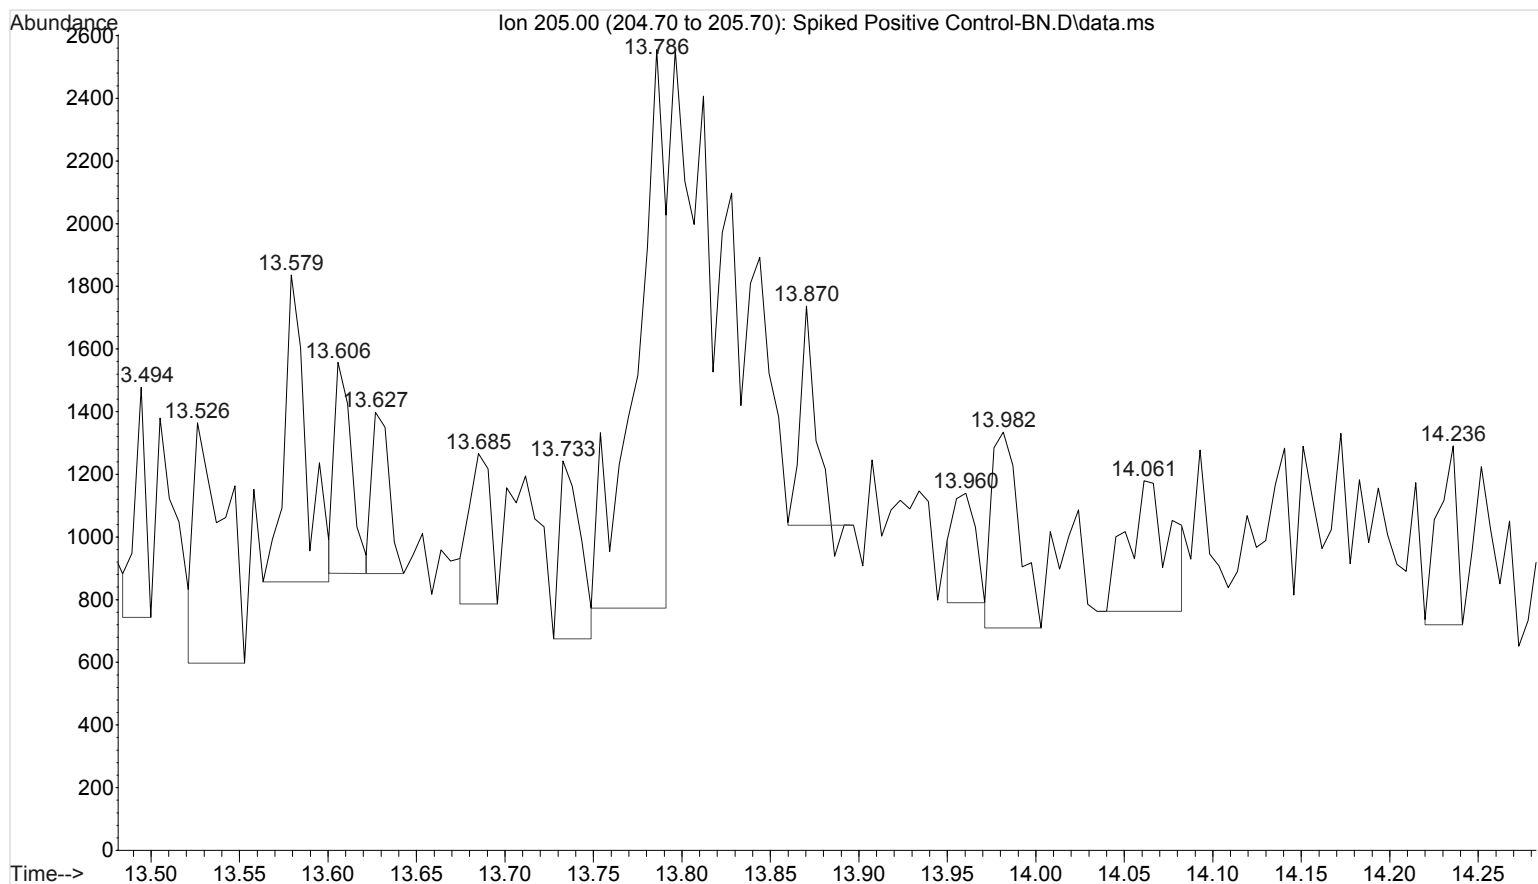

File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \POSTBLK.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 19 Jun 2016 03:30 using AcqMethod BNSB120510.M  
Sample Name: BLK  
Misc Info : Chloroform

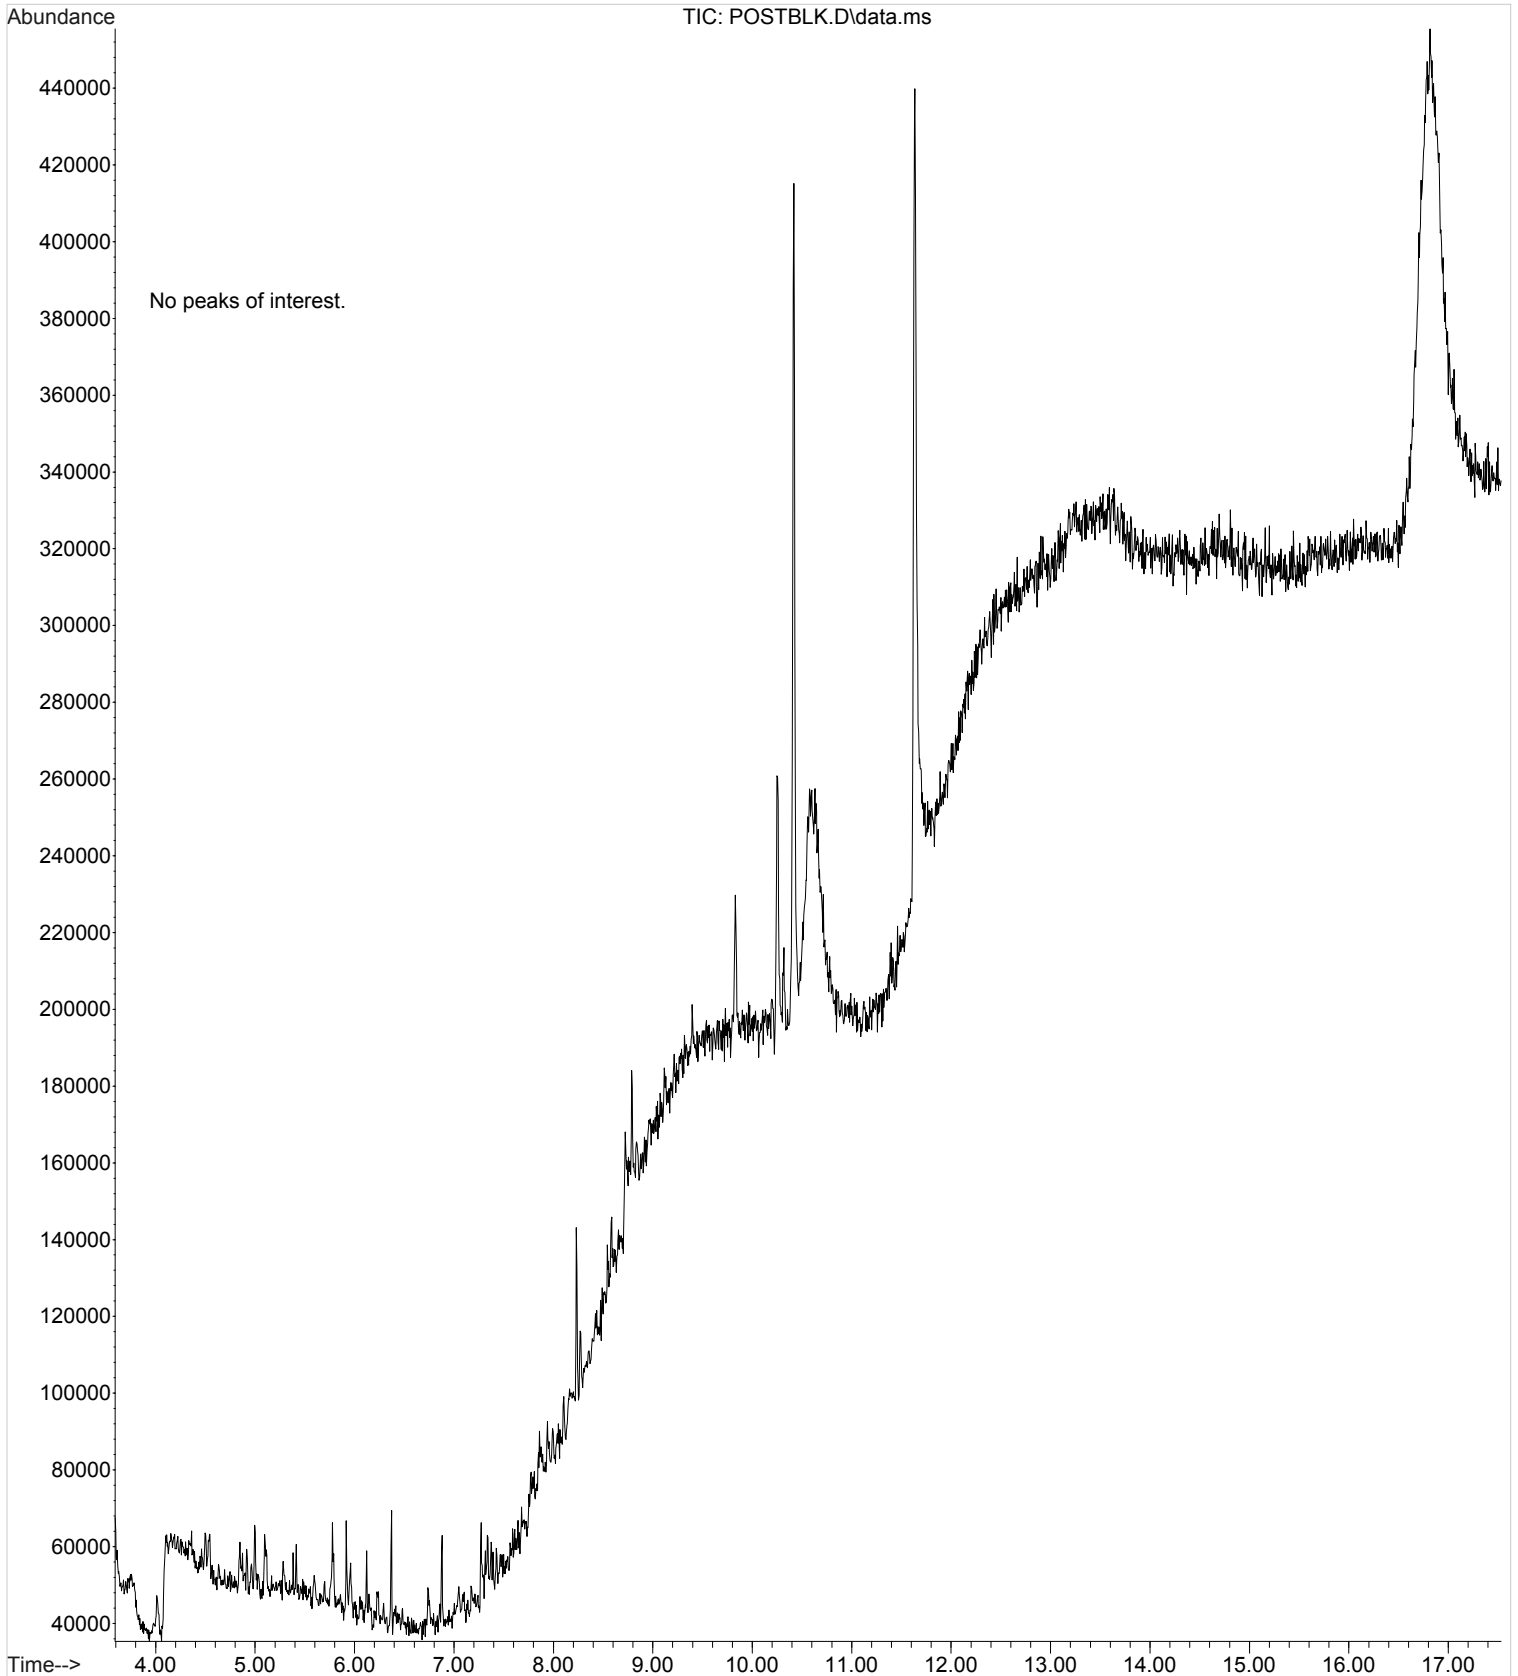

Analytical Method 3.6.1 & 3.6.7 QA Check List

---

Run Start Date: 06/16/2016

Analyst: CS

(Long GC/MS temperature program)

Positive Control Compound List


- Phentermine
- Methamphetamine
- Nicotine
- Meperidine
- Caffeine
- Diphenhydramine
- Lidocaine
- PCP
- Methadone
- Amitriptyline
- Codeine
- Trazodone

Internal Standards


- Benzphetamine
- Papaverine

Optional back extraction **not** performed.  
Reconstituted in MeOH.


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Prerun Solvent Blankr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 14:20 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Pre-run Solvent Blank  
Misc Info : Chloroform

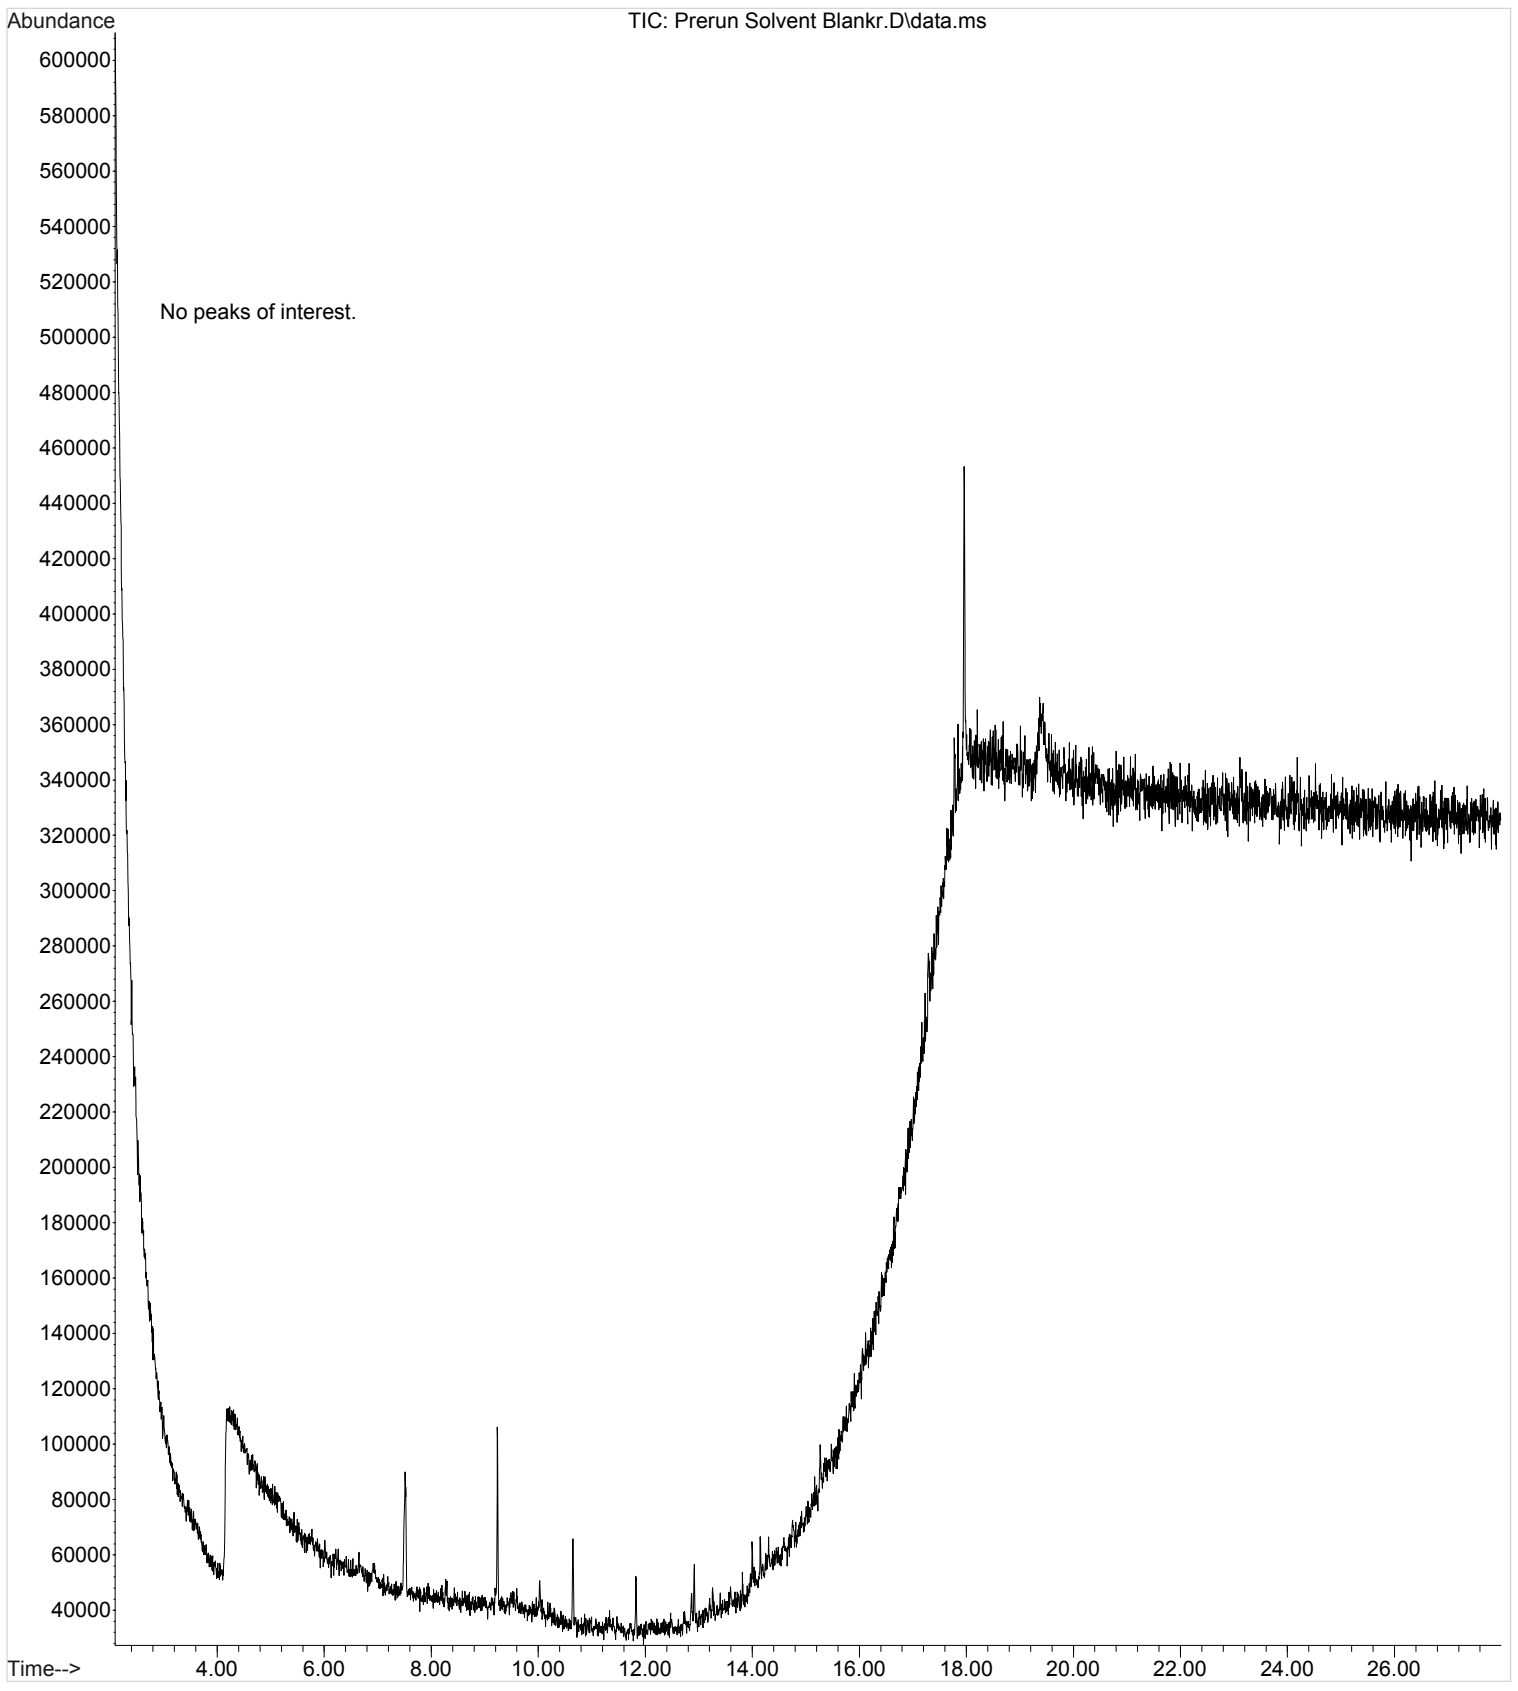



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \prbLK2r.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 16:01 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Solvent Blank  
Misc Info : Chloroform

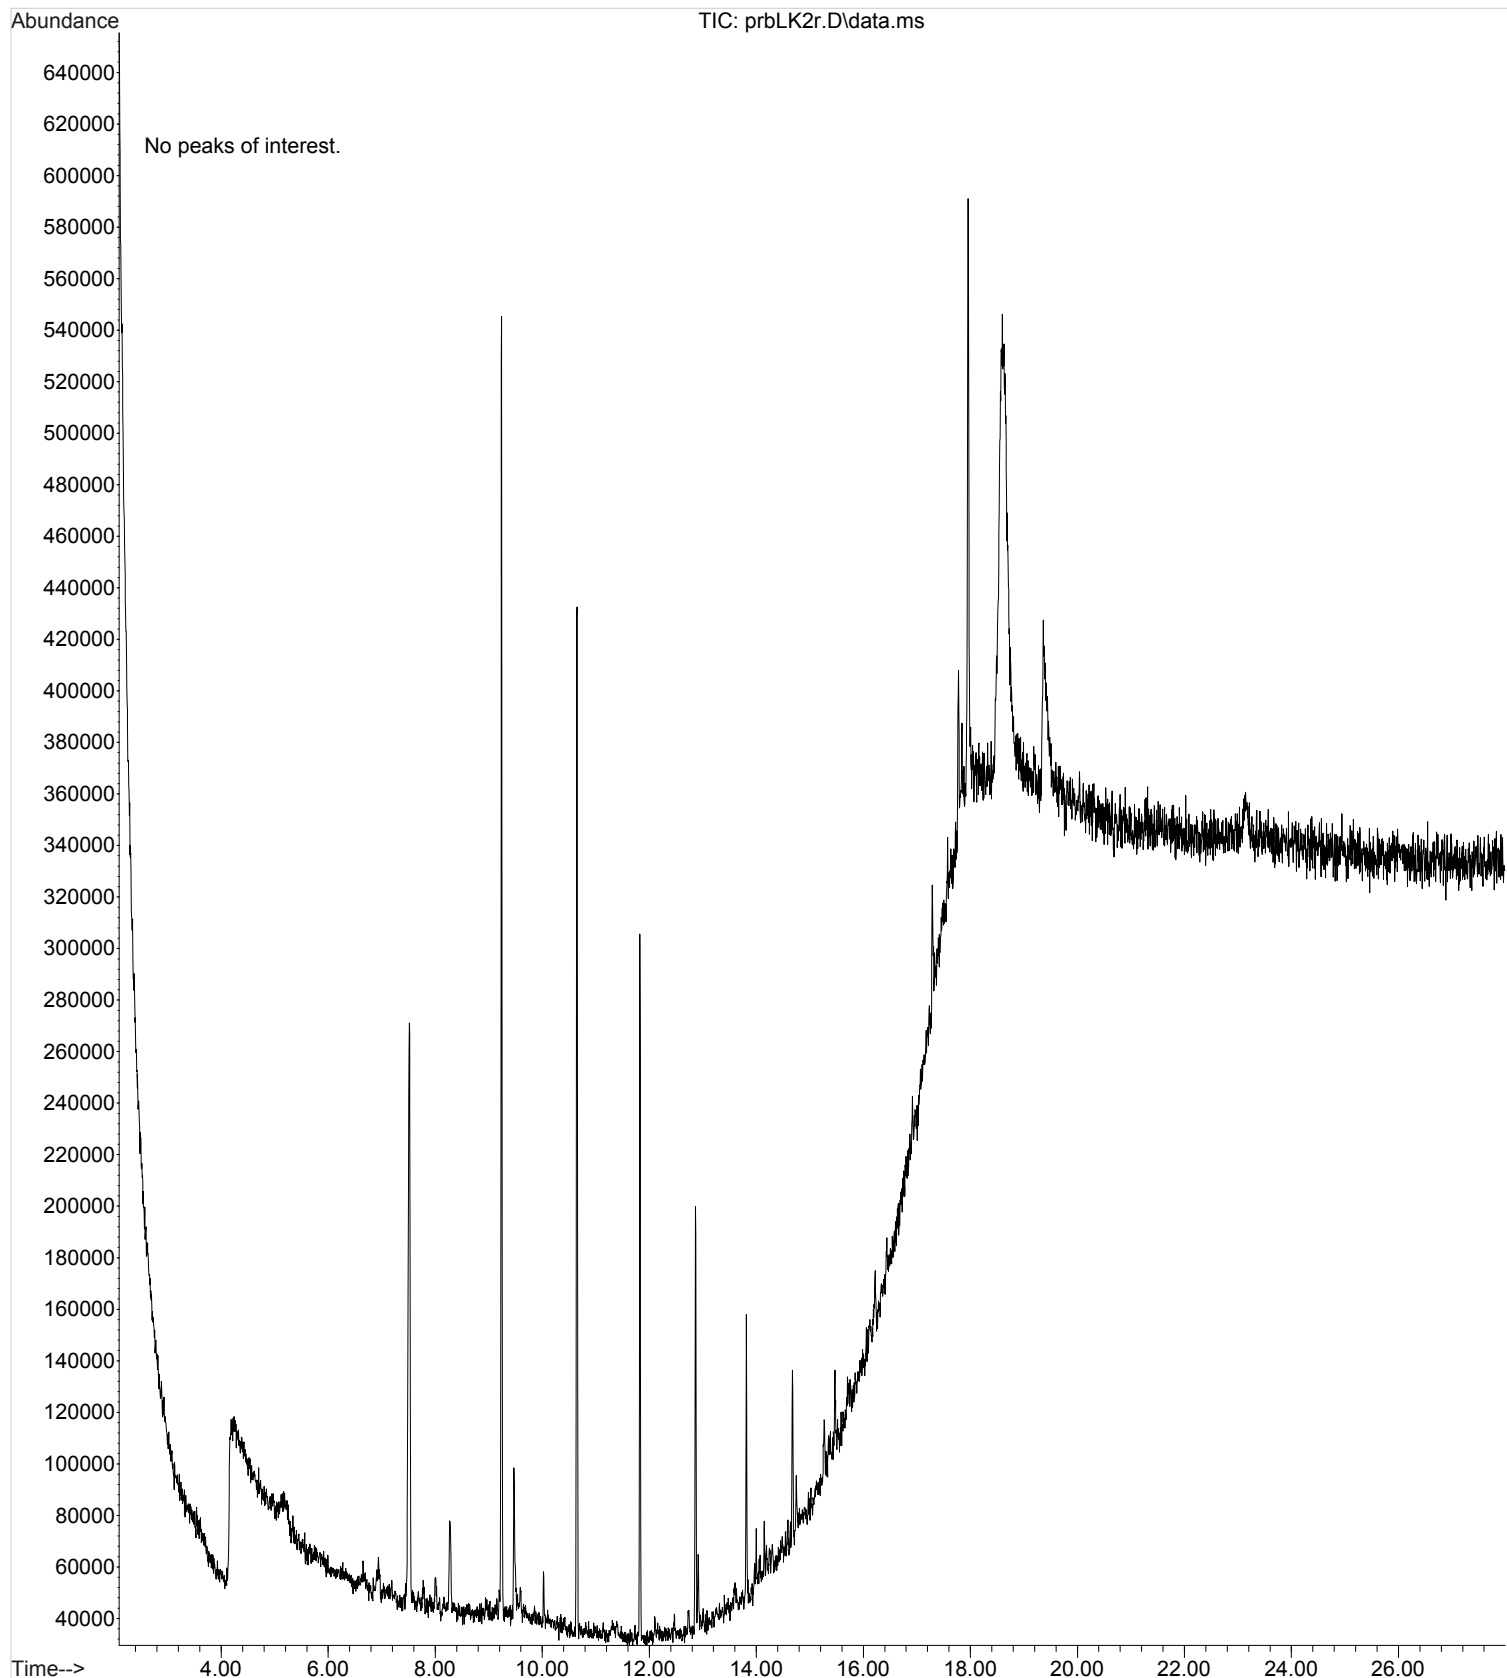

File :I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Negative Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 14:54 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Negative Control - Utak Lot B1013  
Misc Info : Analytical Method 3.6.1


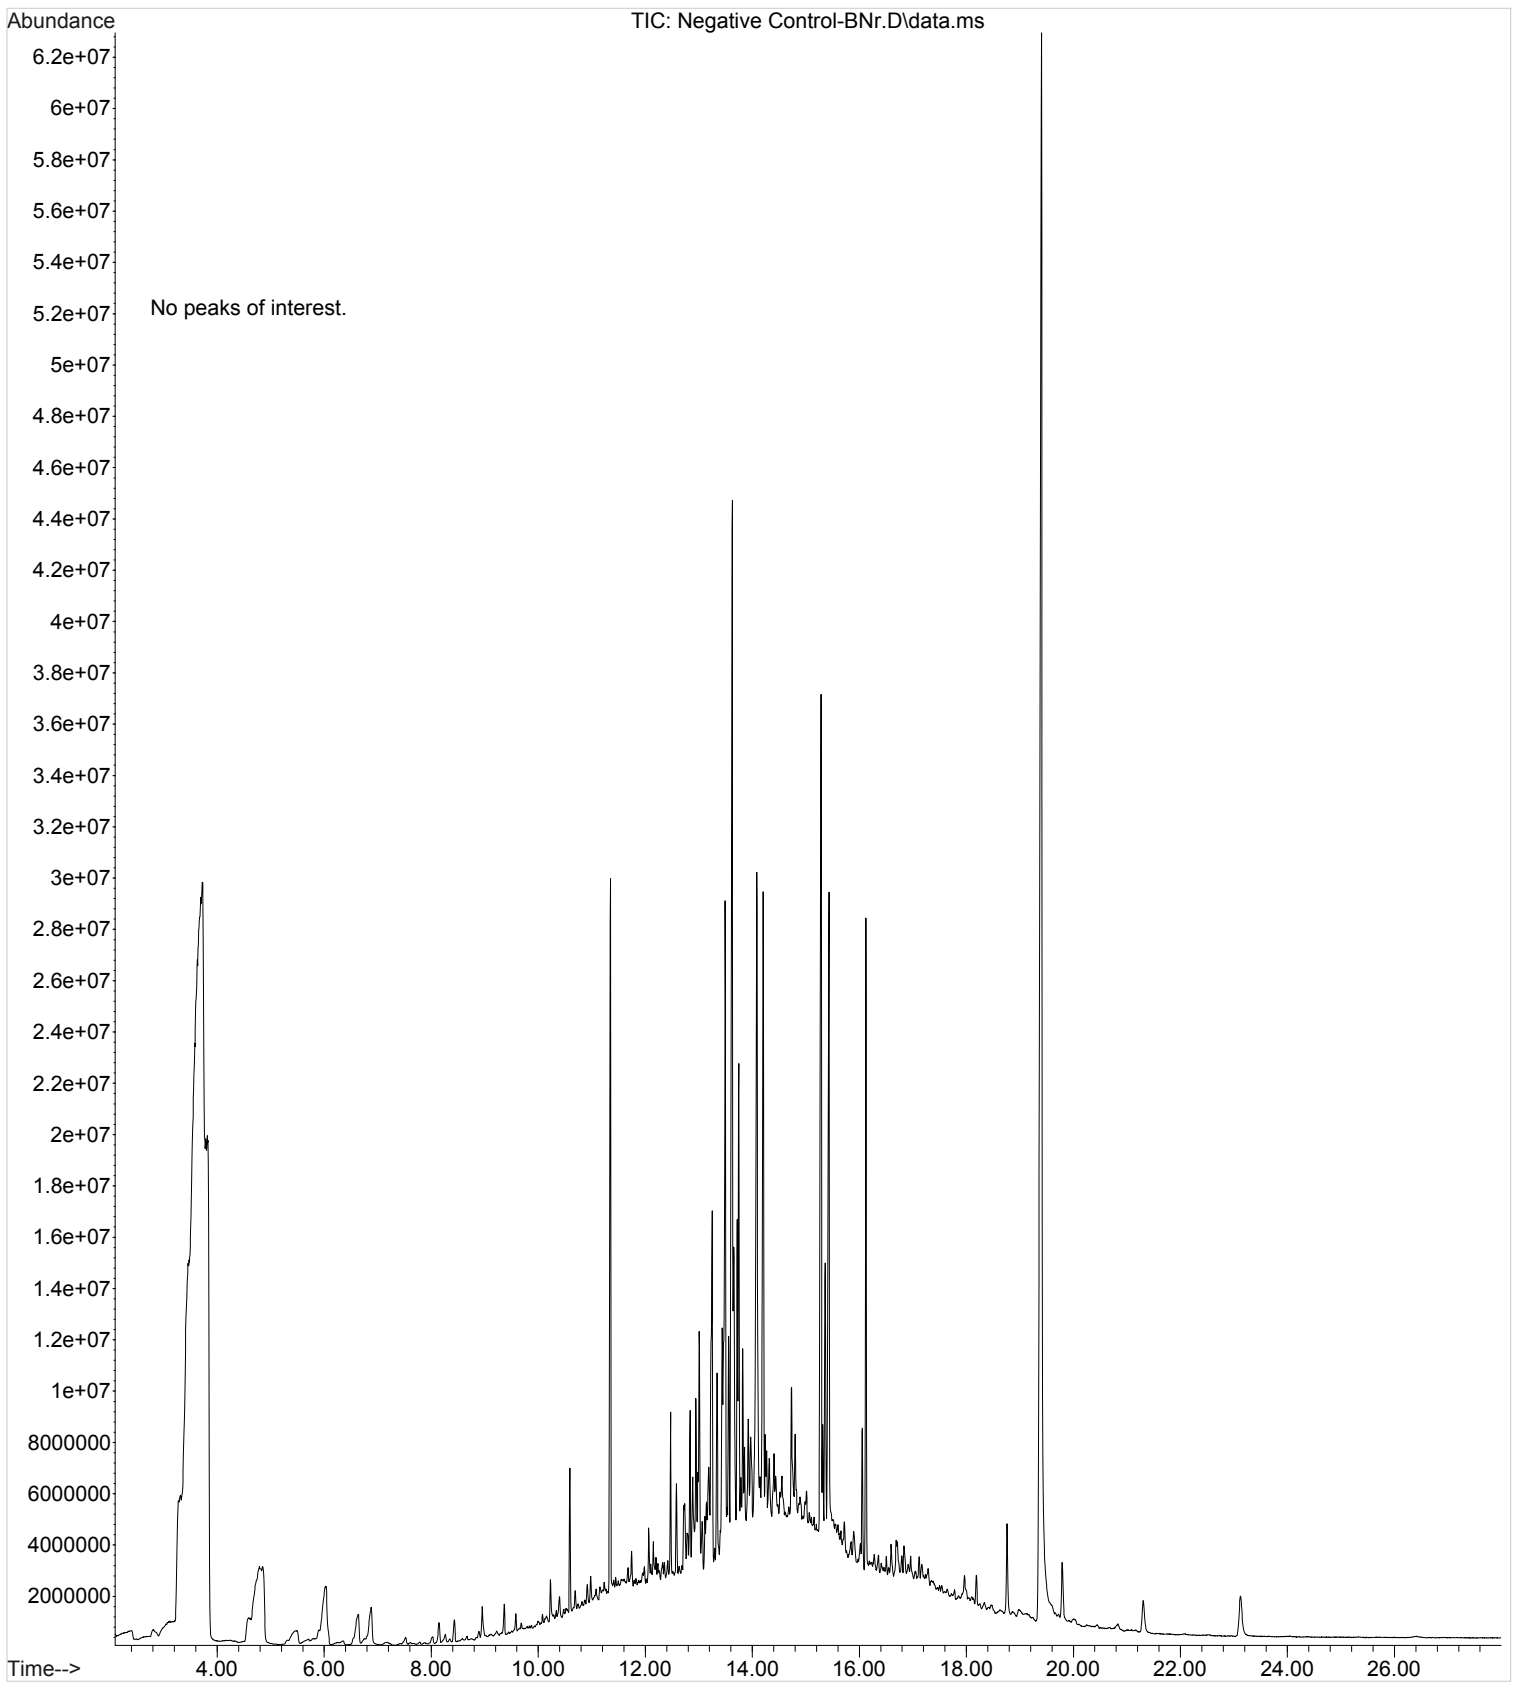


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Negative Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 14:54 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Negative Control - Utak Lot B1013  
Misc Info : Analytical Method 3.6.1

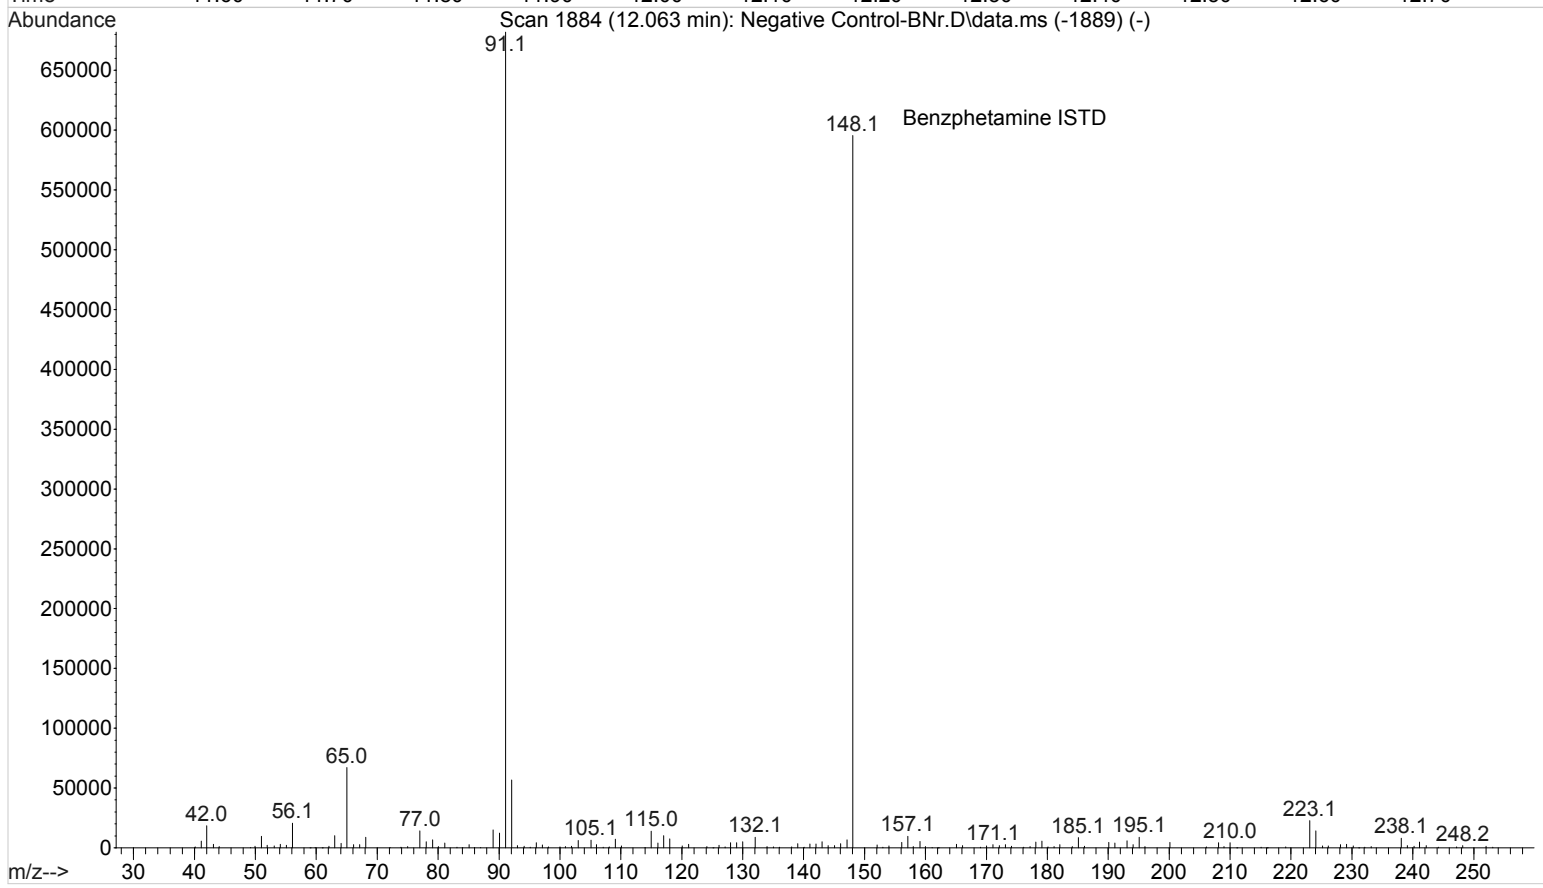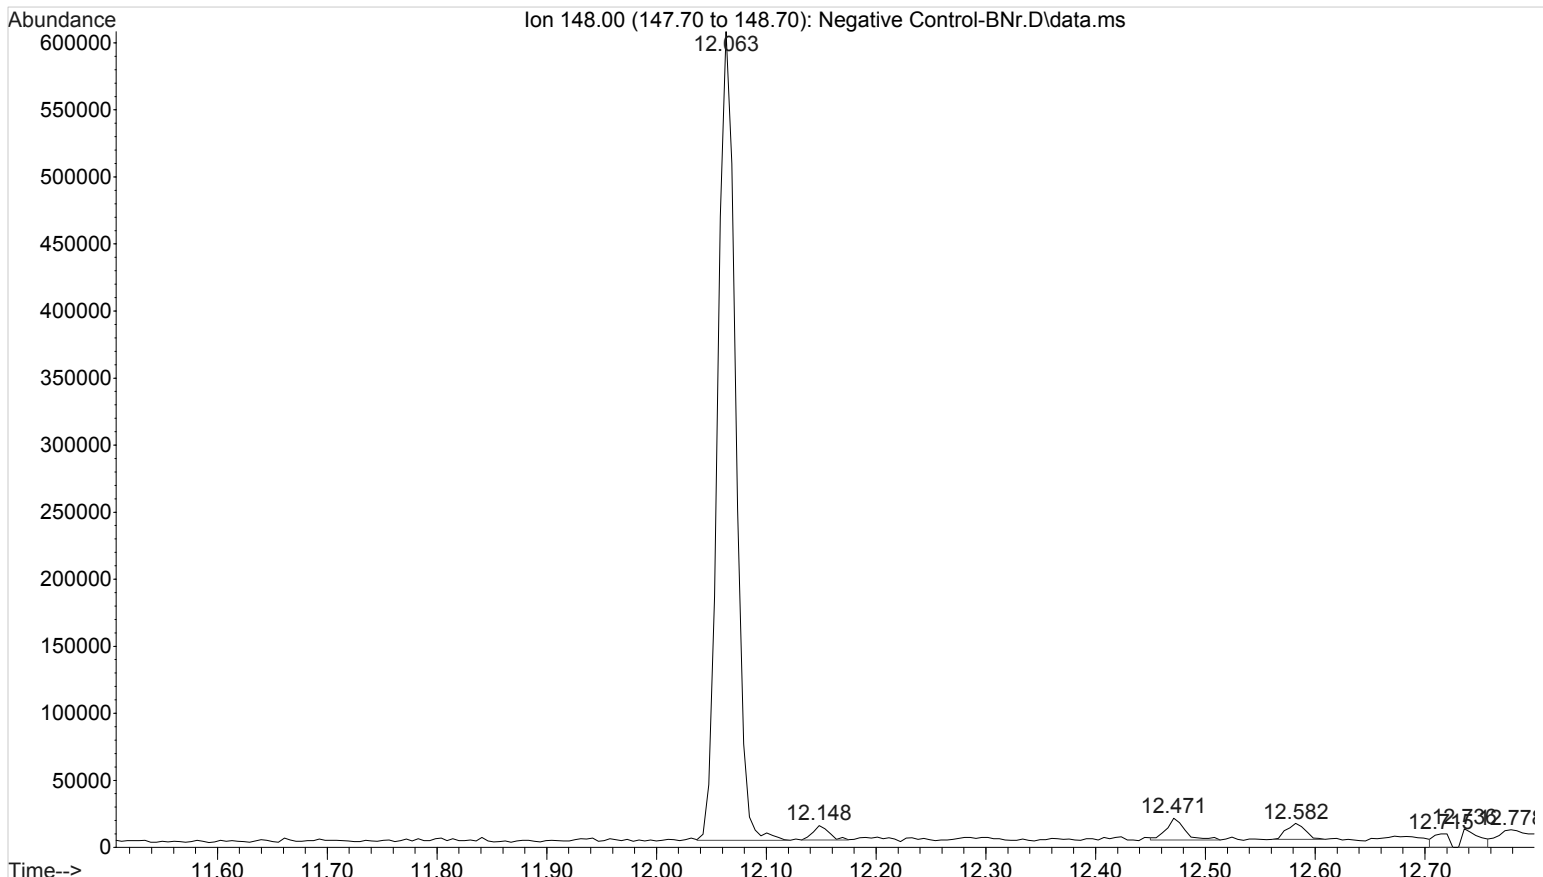






File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Negative Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 14:54 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Negative Control - Utak Lot B1013  
Misc Info : Analytical Method 3.6.1

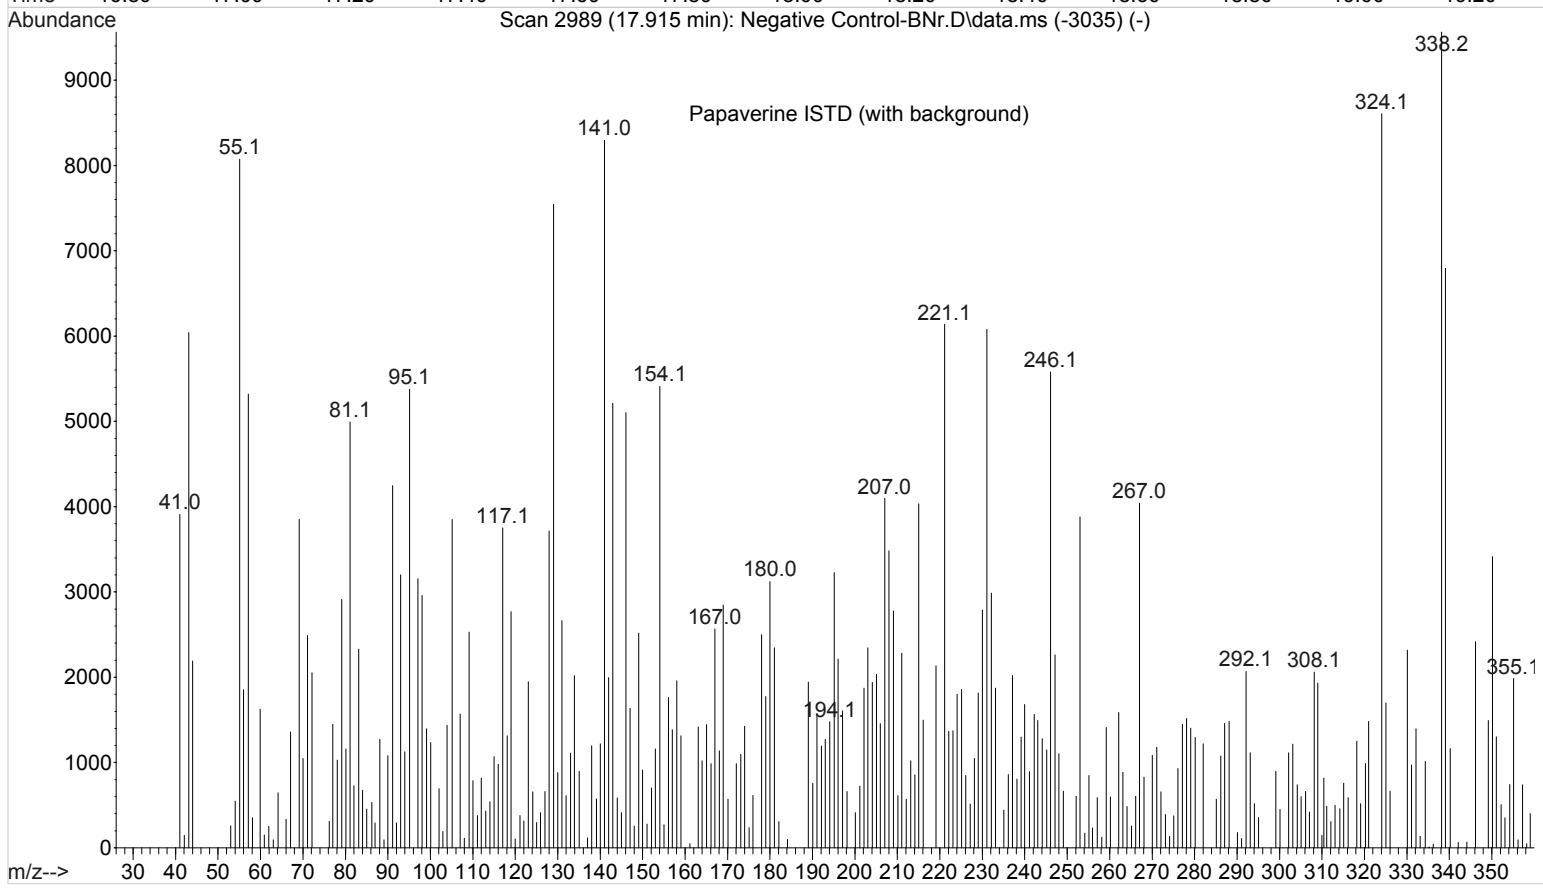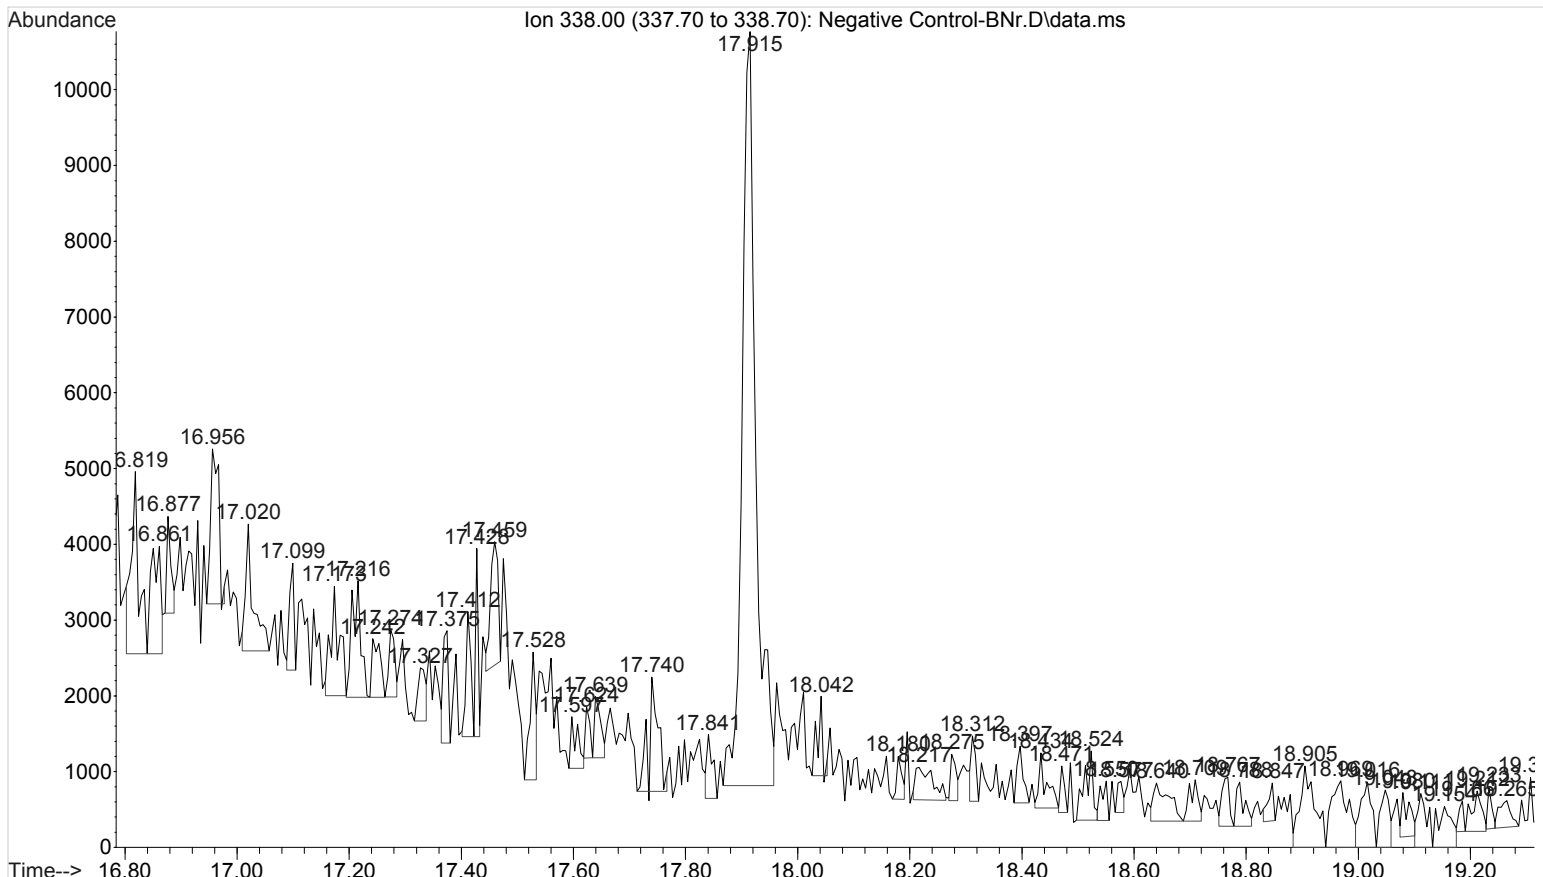



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Spiked Positive Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 15:27 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

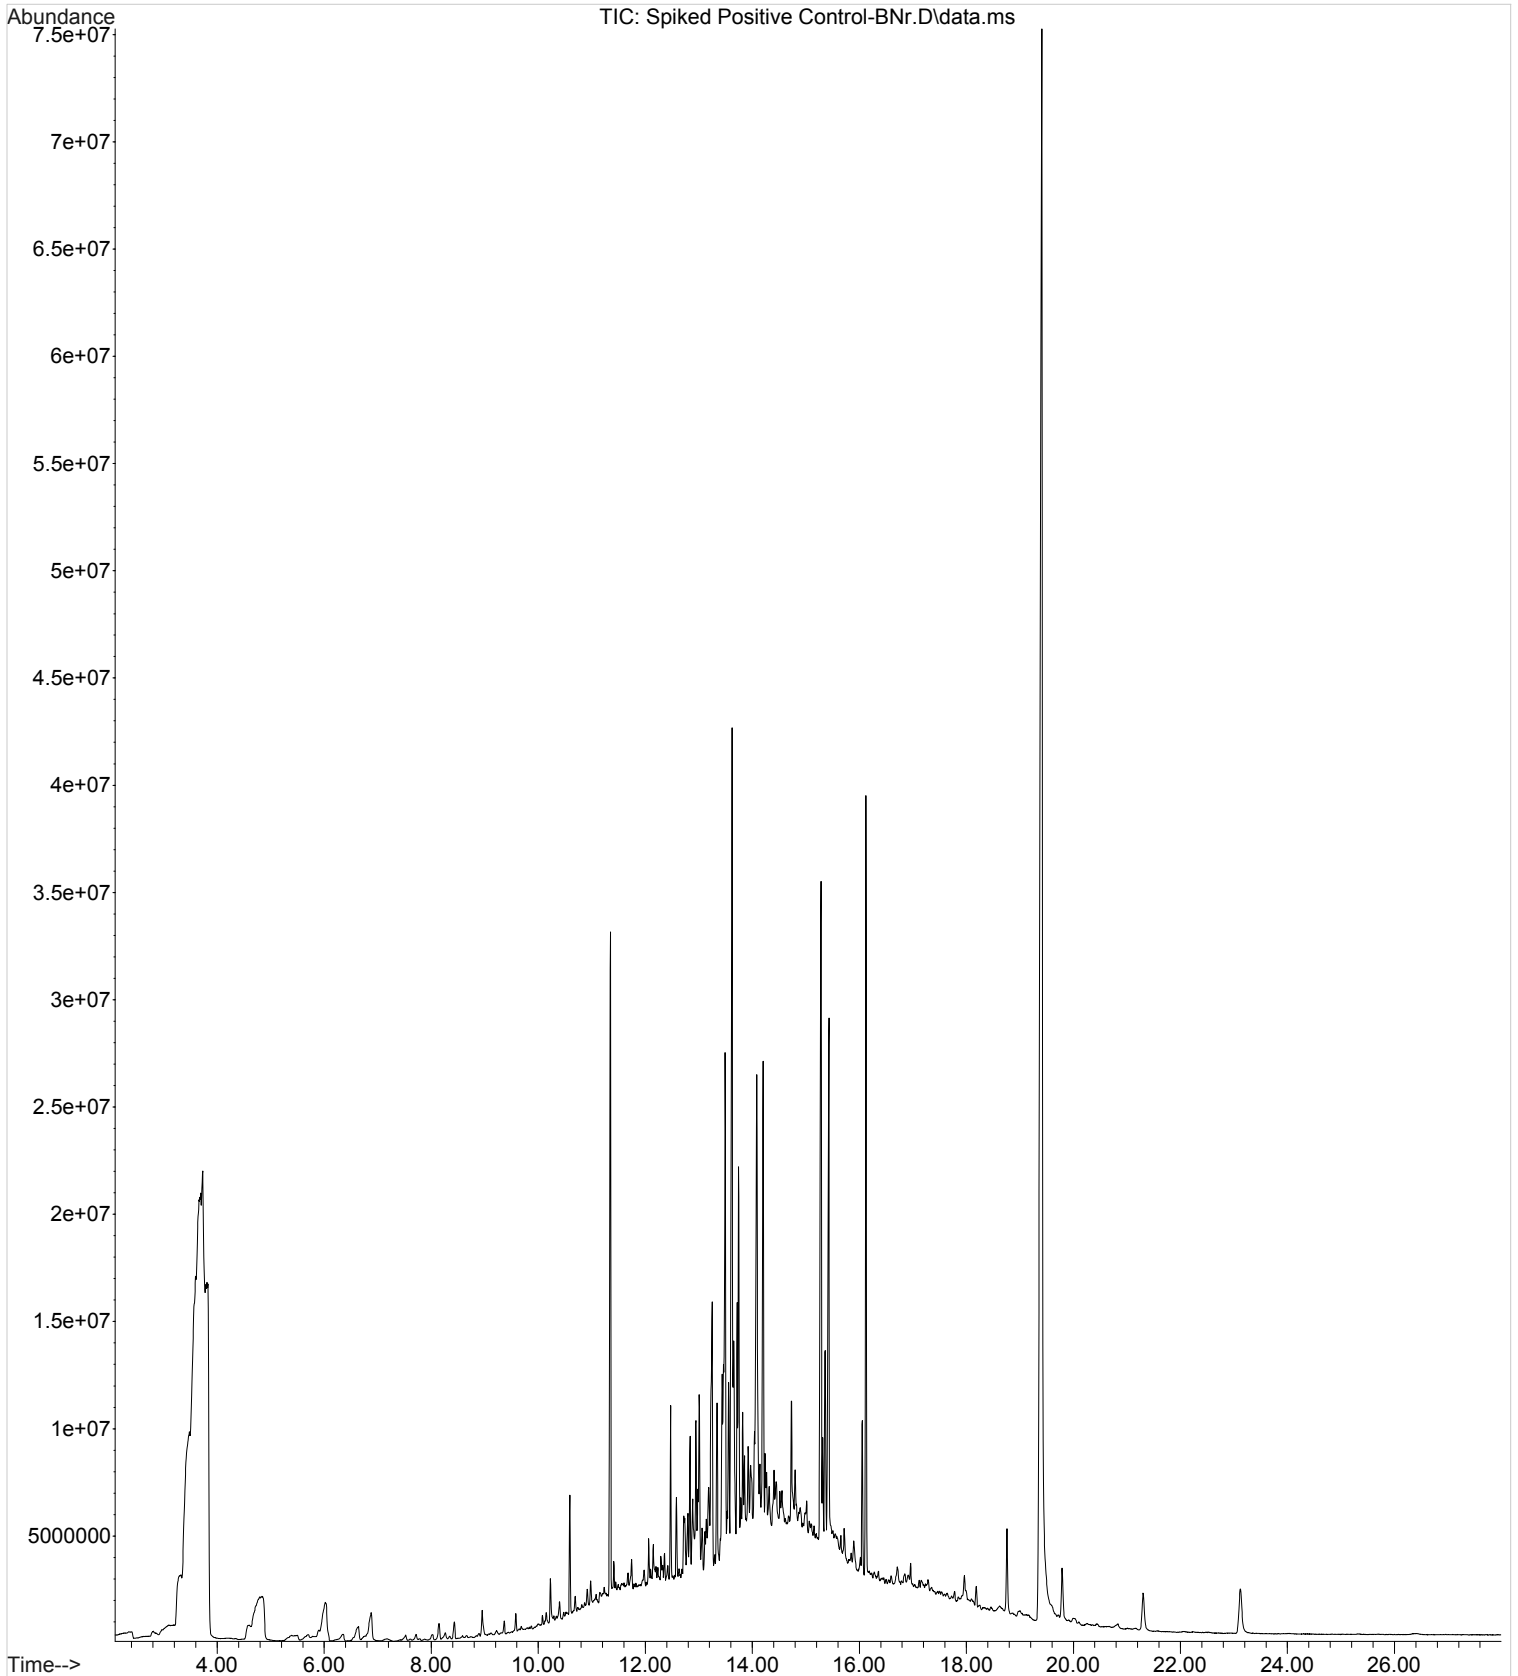



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Spiked Positive Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 15:27 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

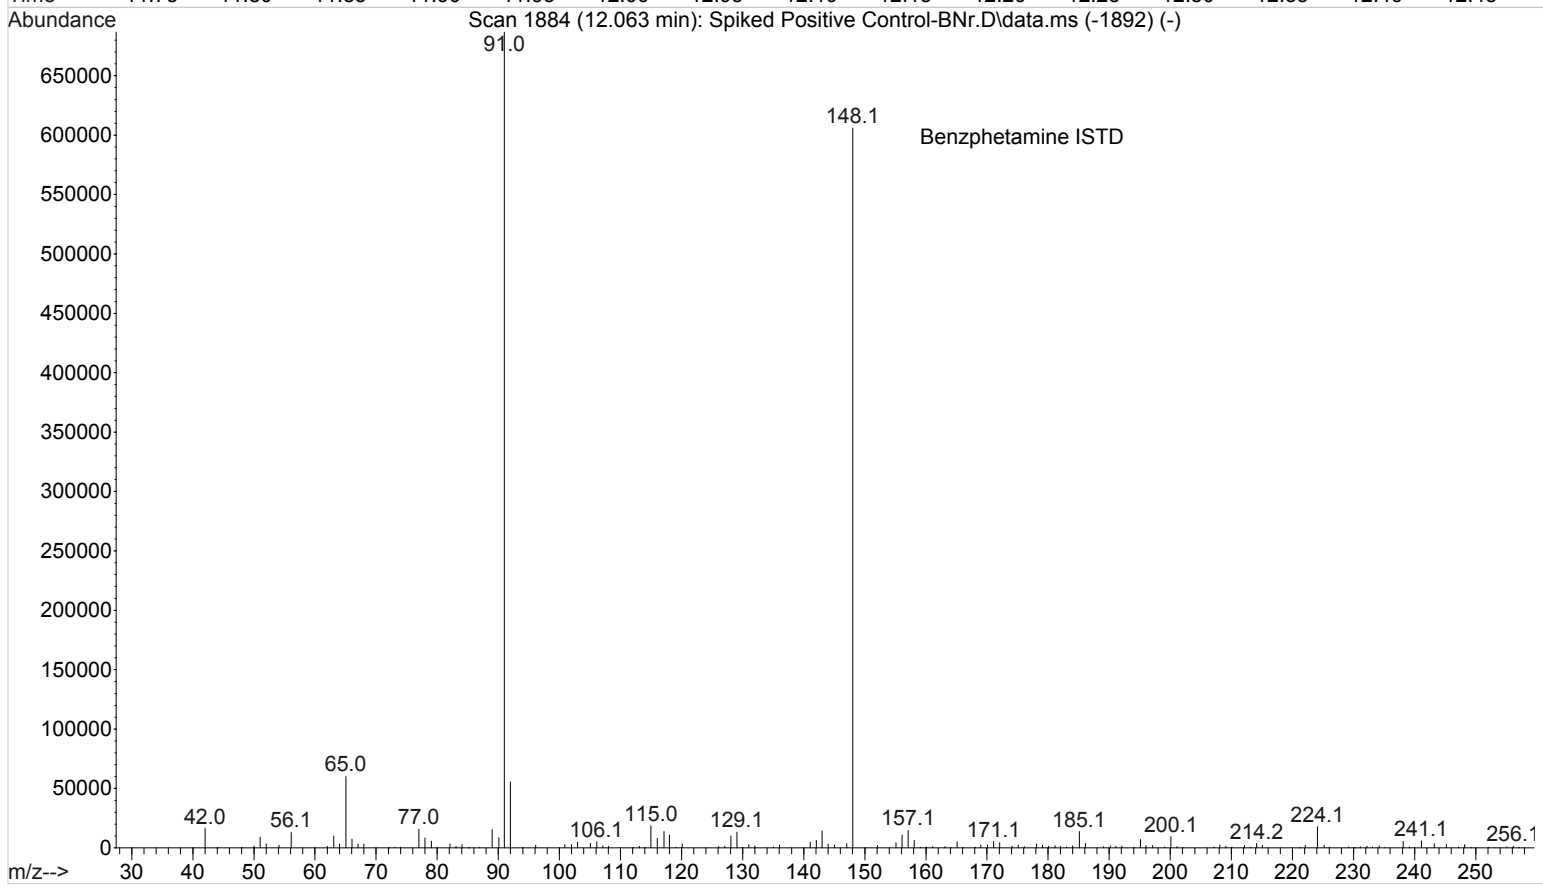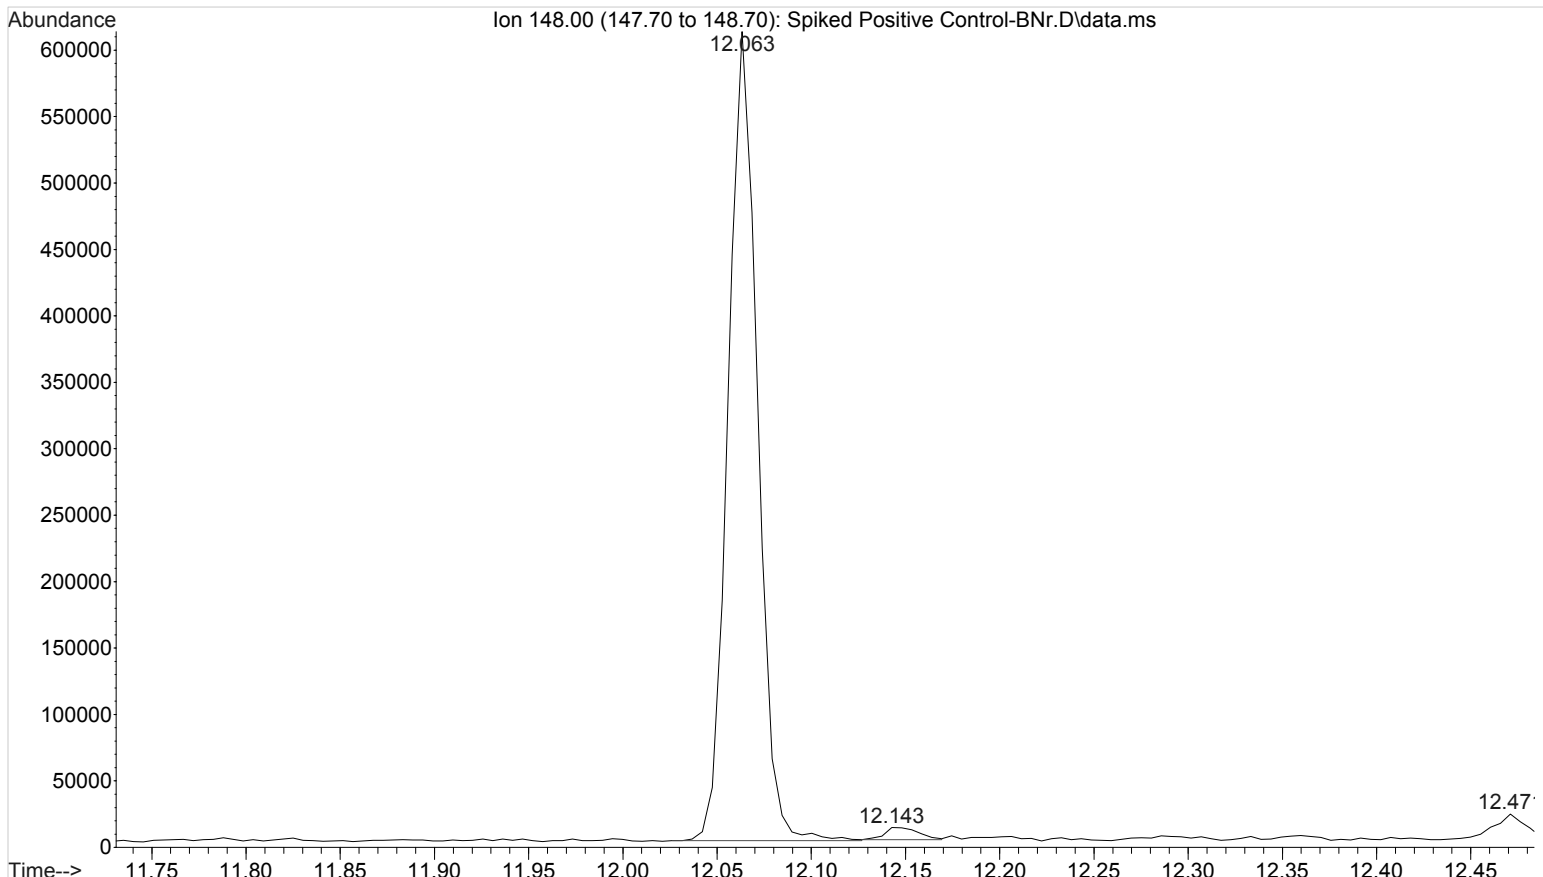



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Spiked Positive Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 15:27 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

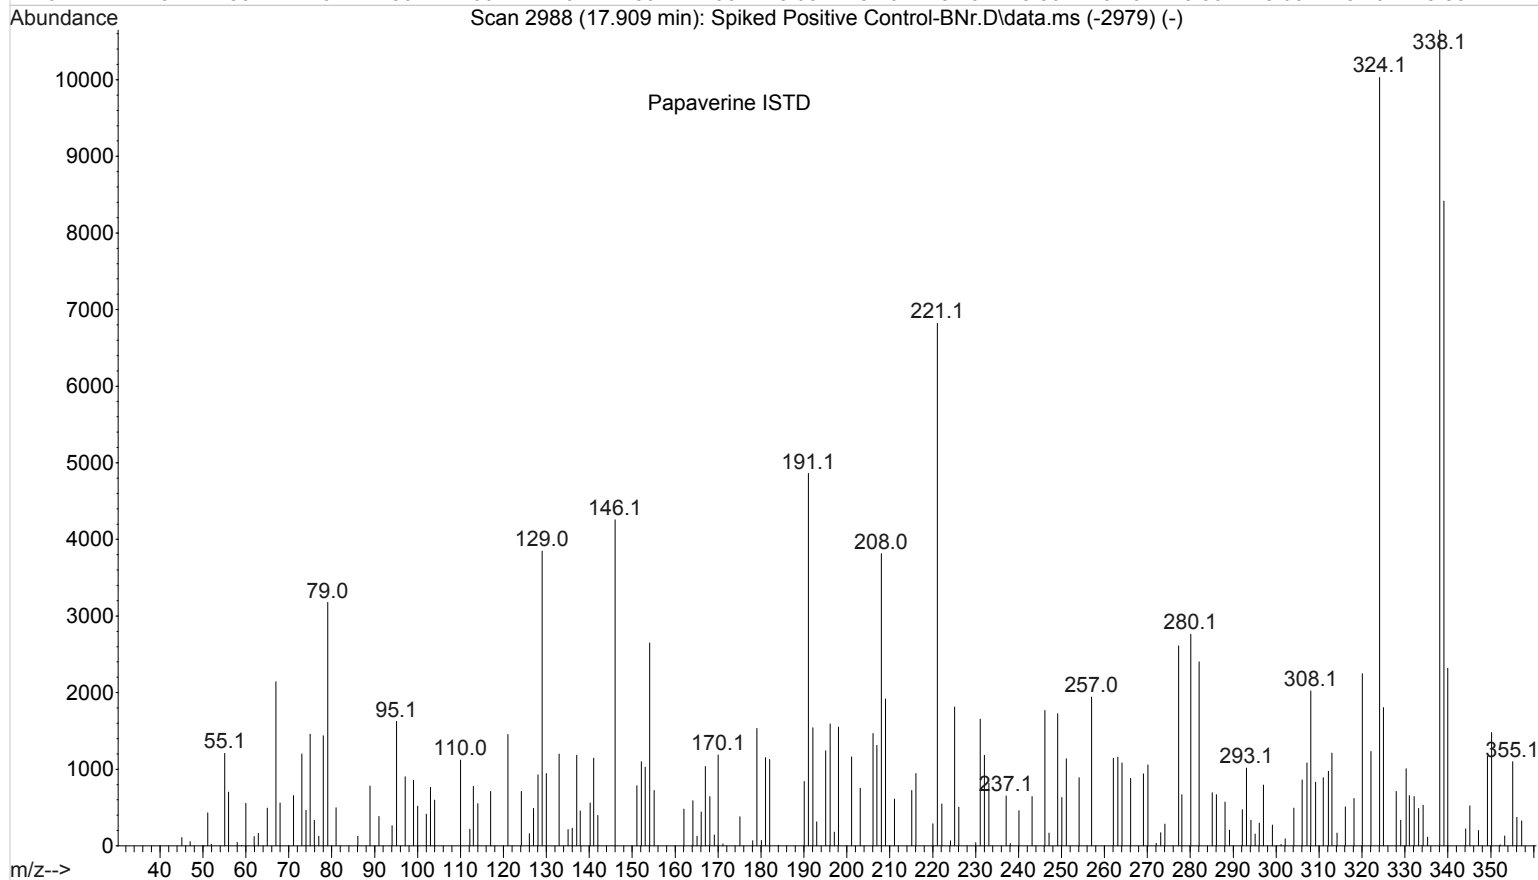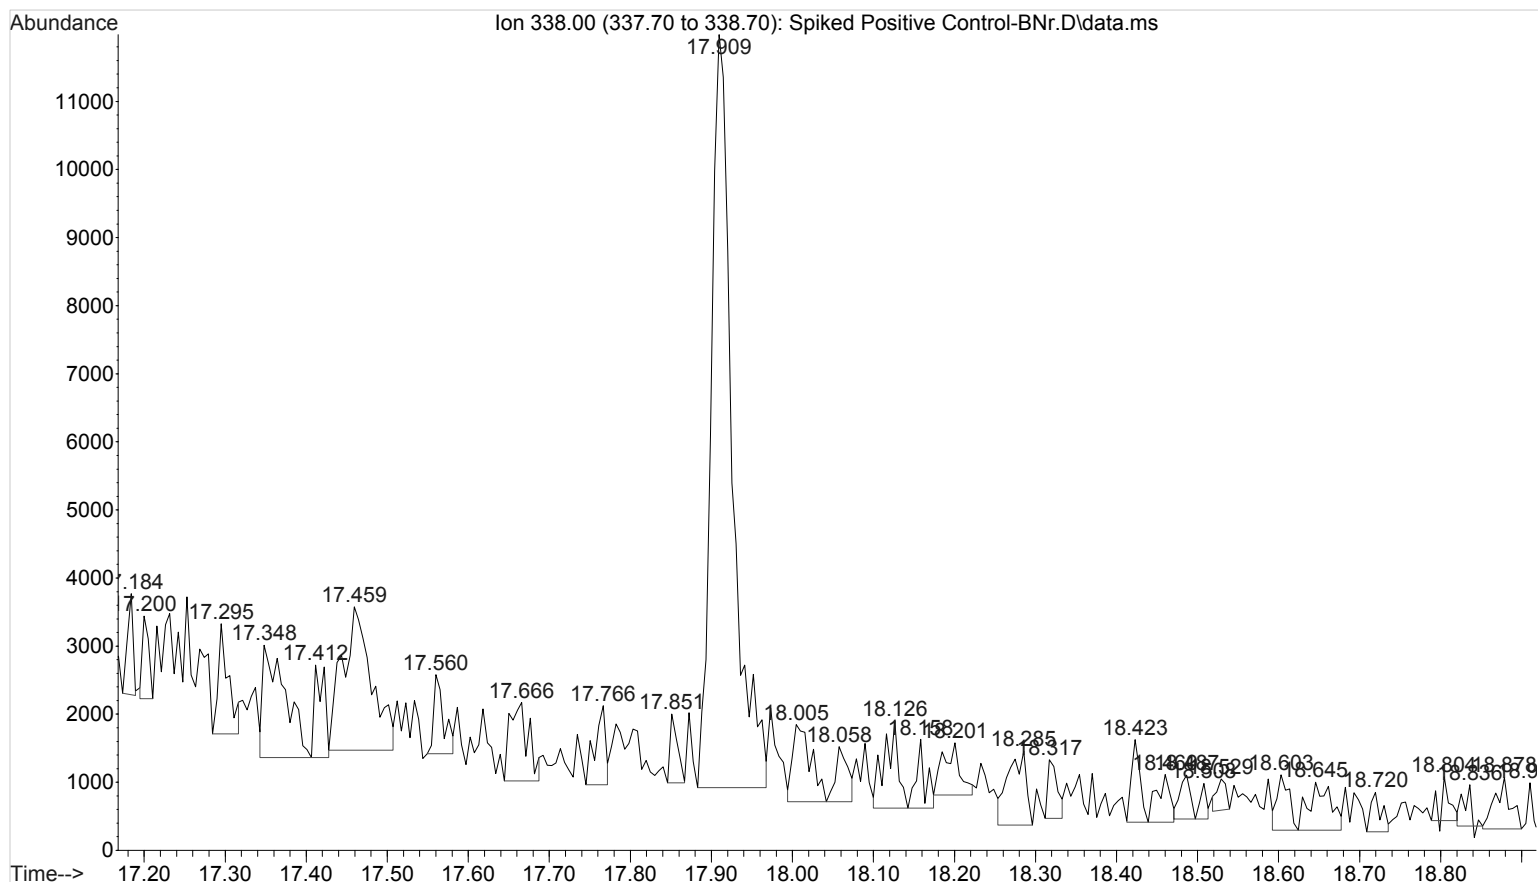



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Spiked Positive Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 15:27 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

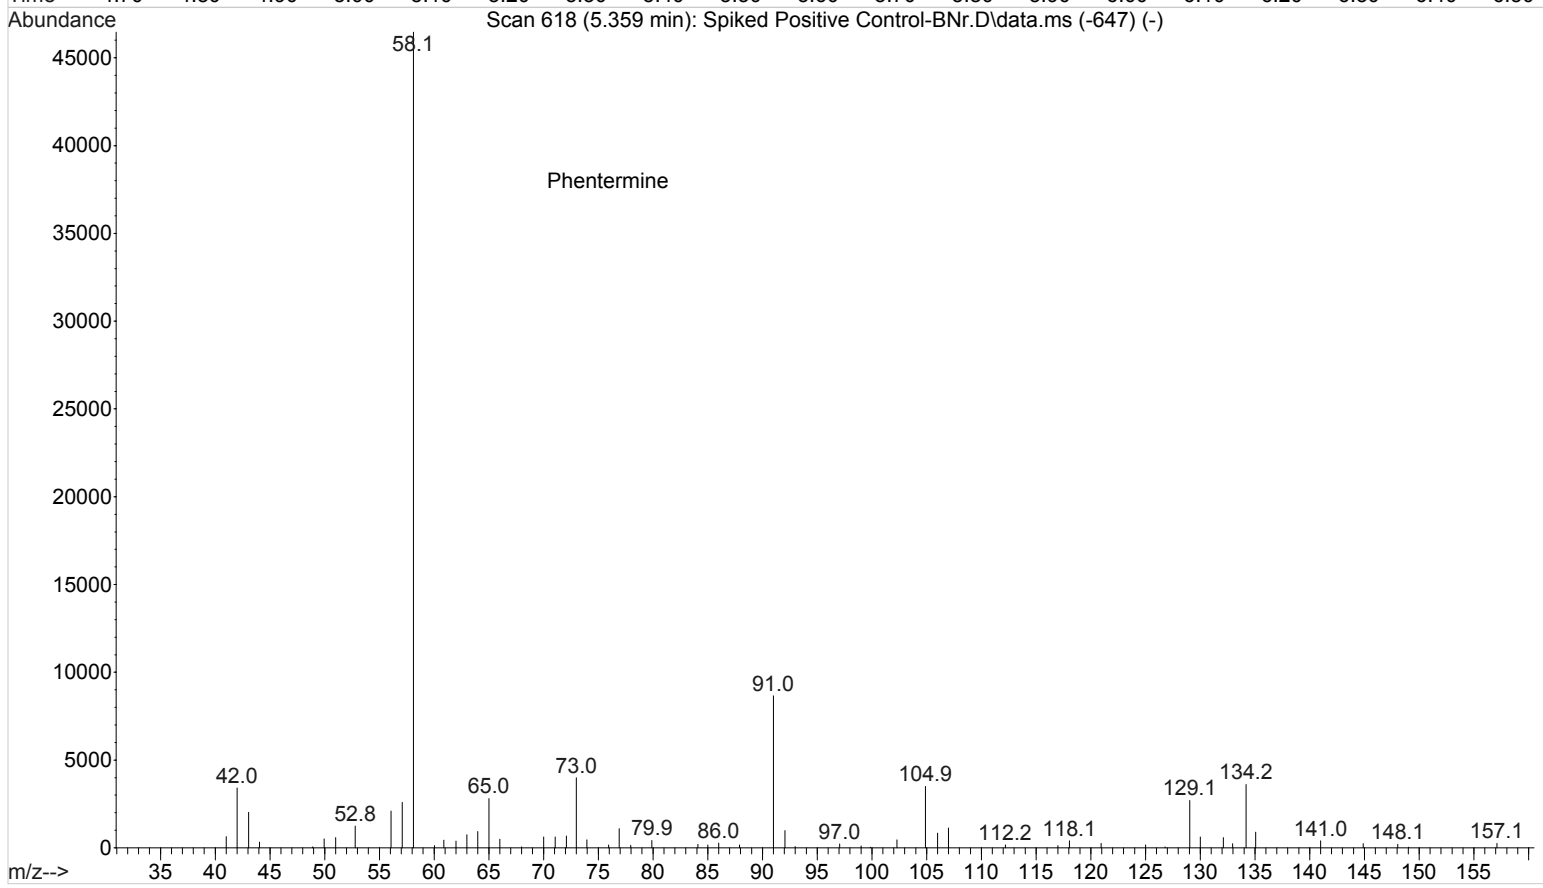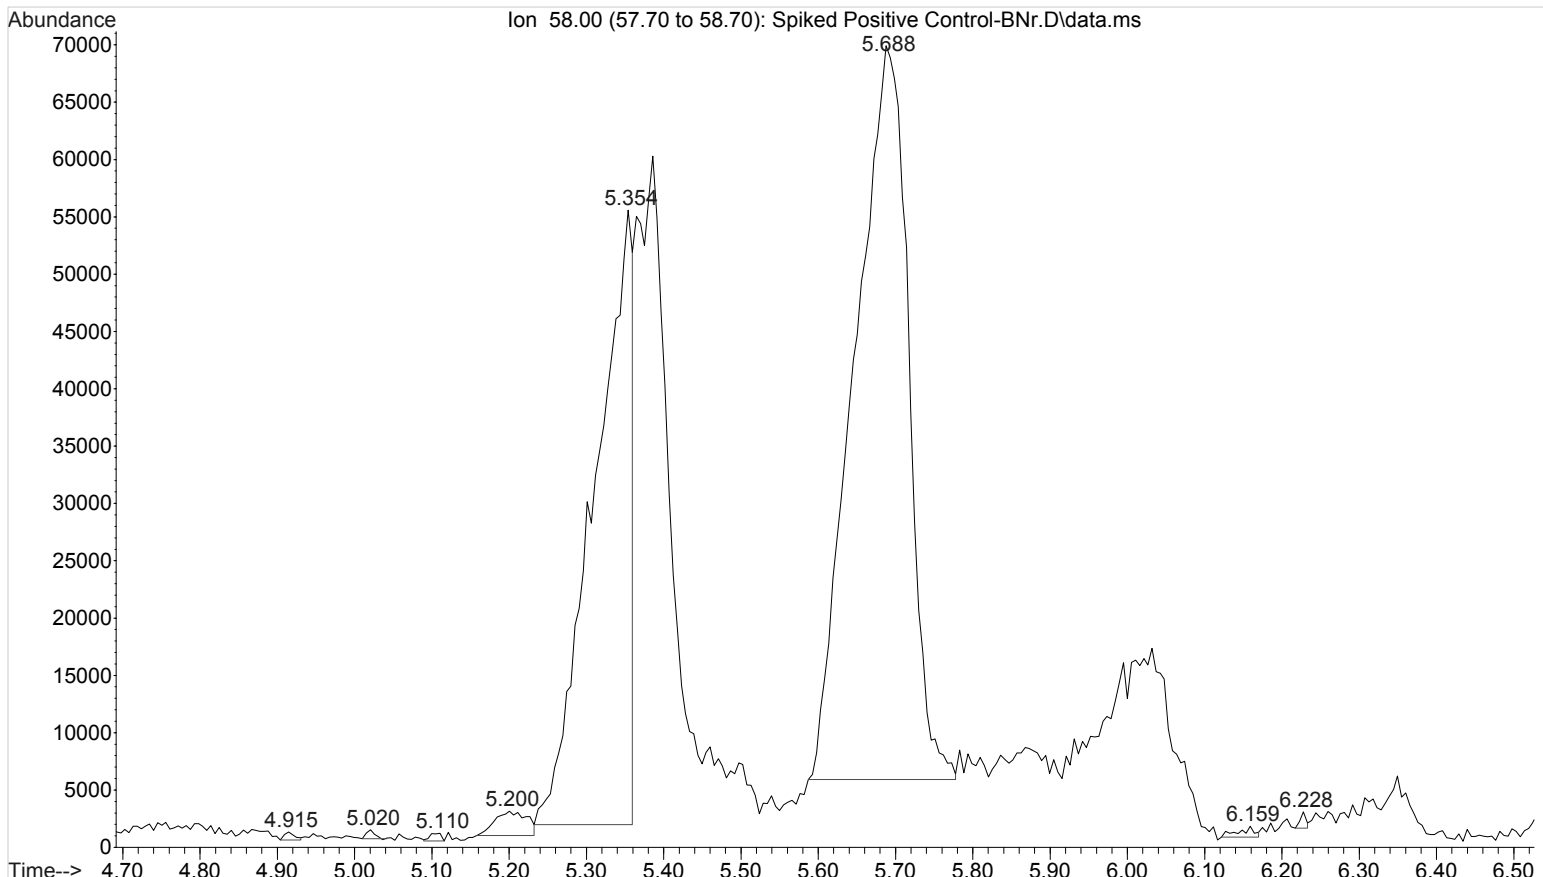



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Spiked Positive Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 15:27 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

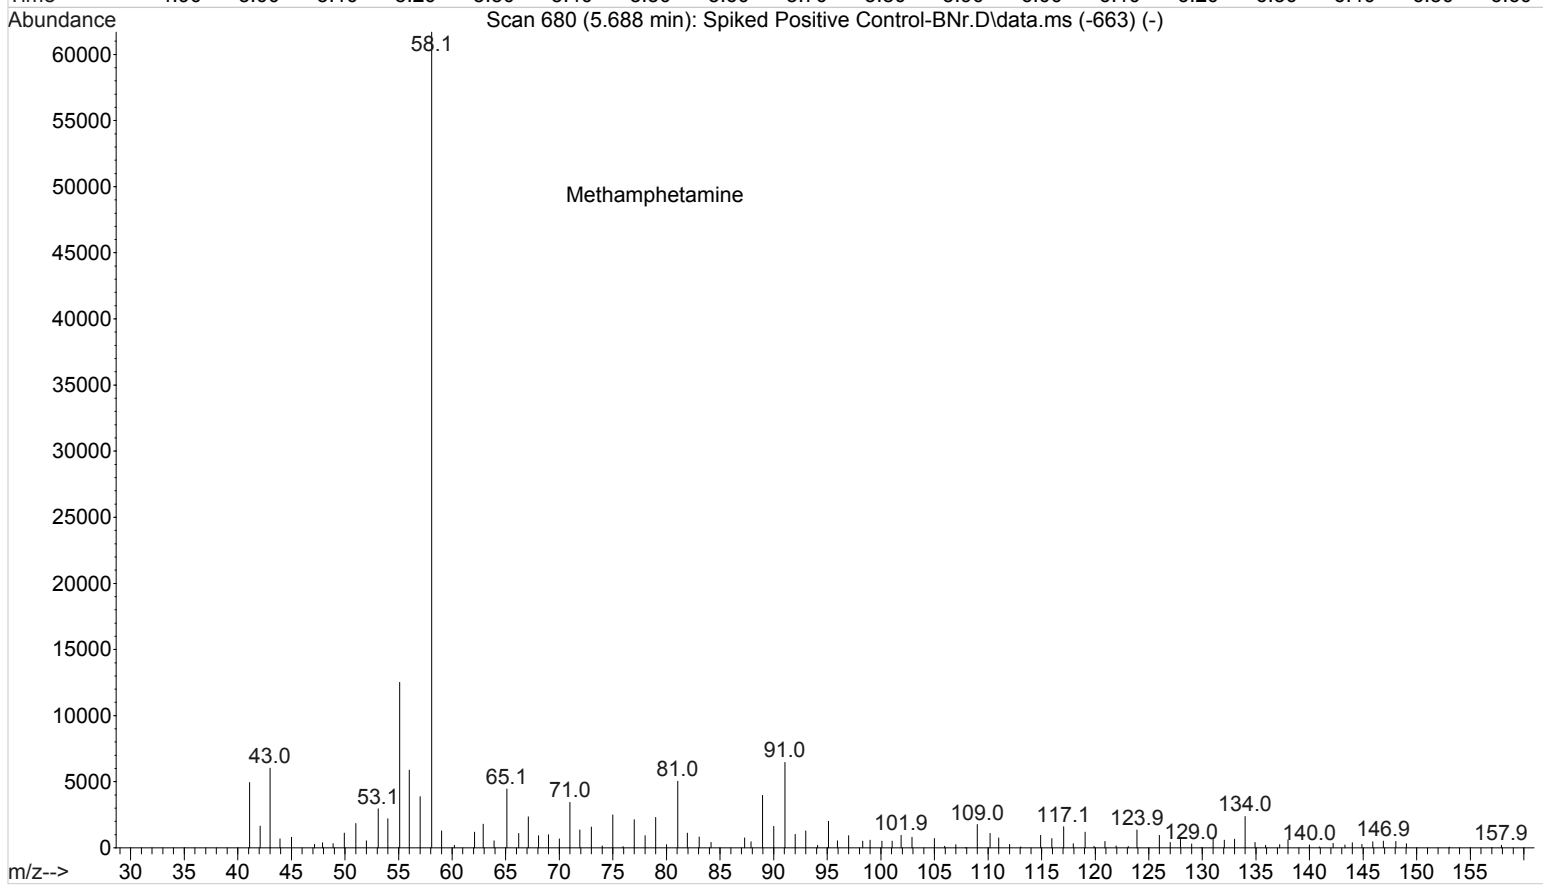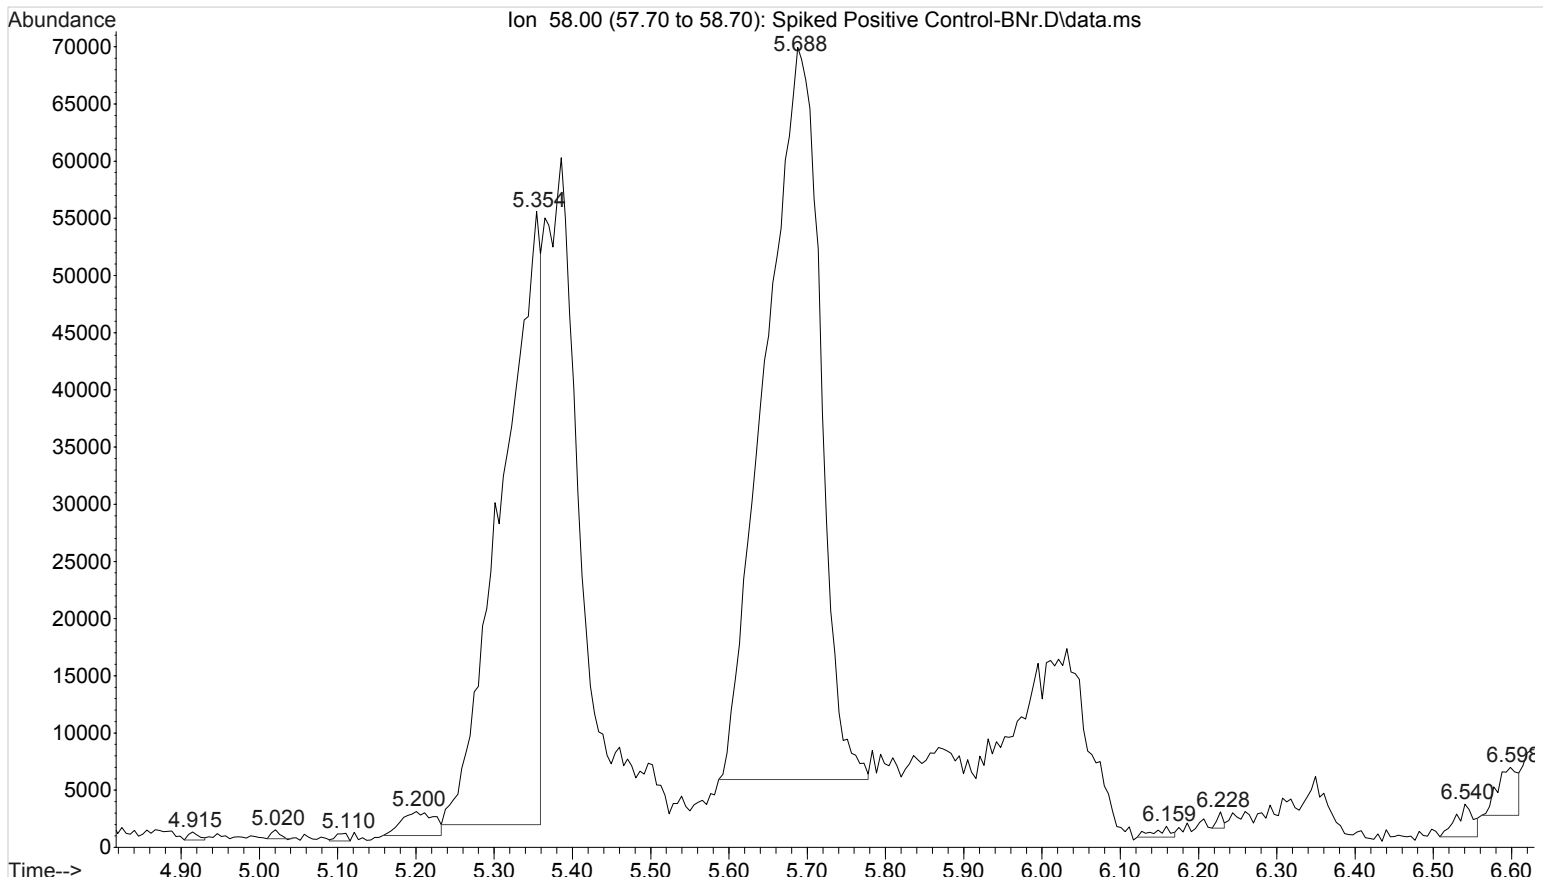

File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Spiked Positive Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 15:27 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

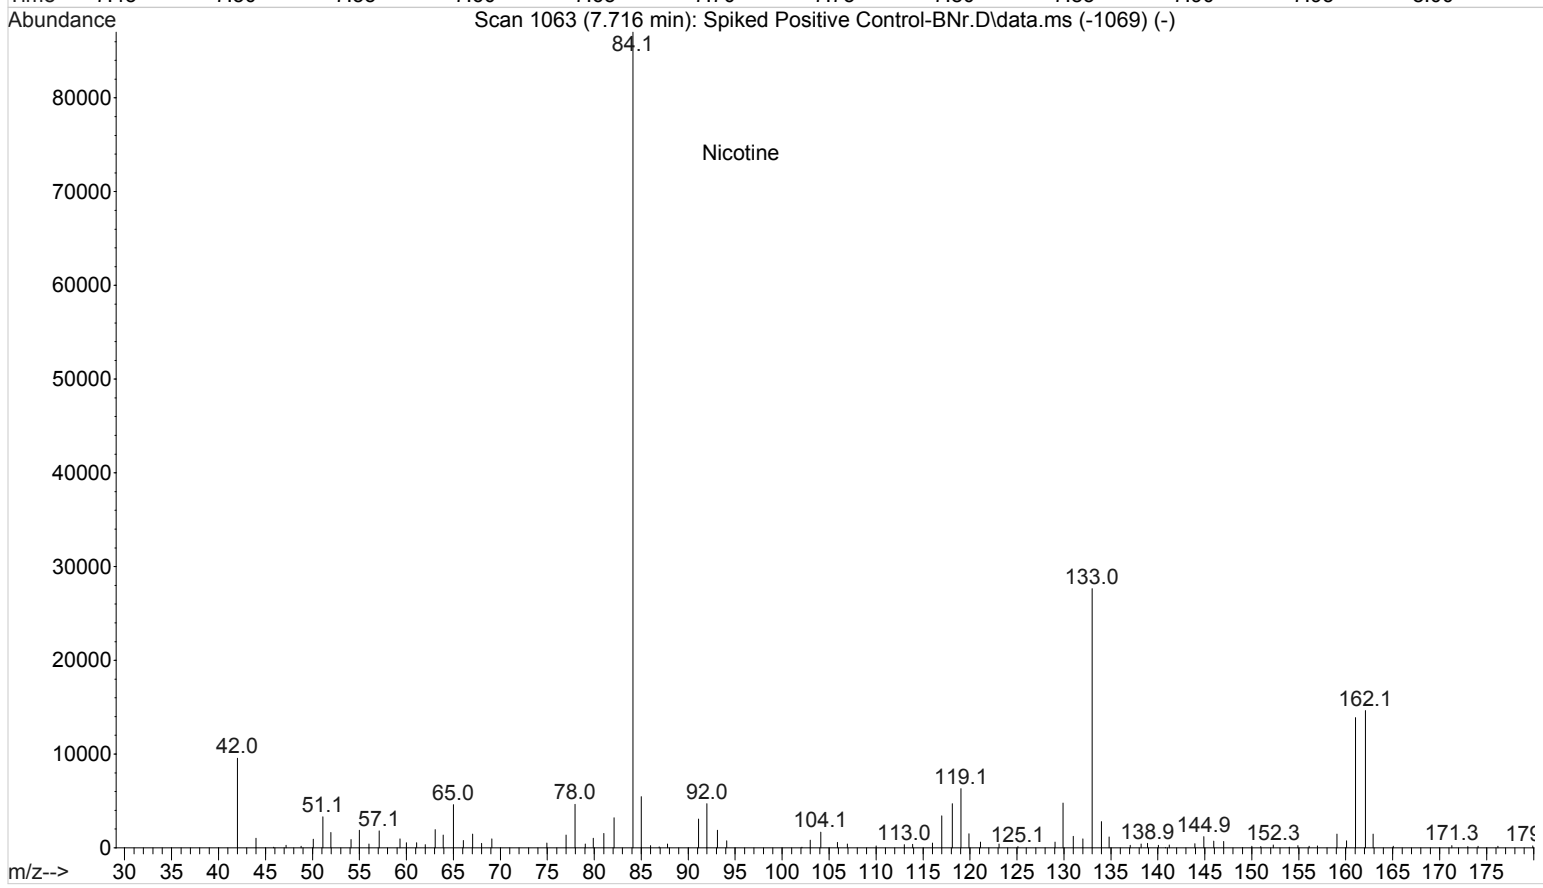
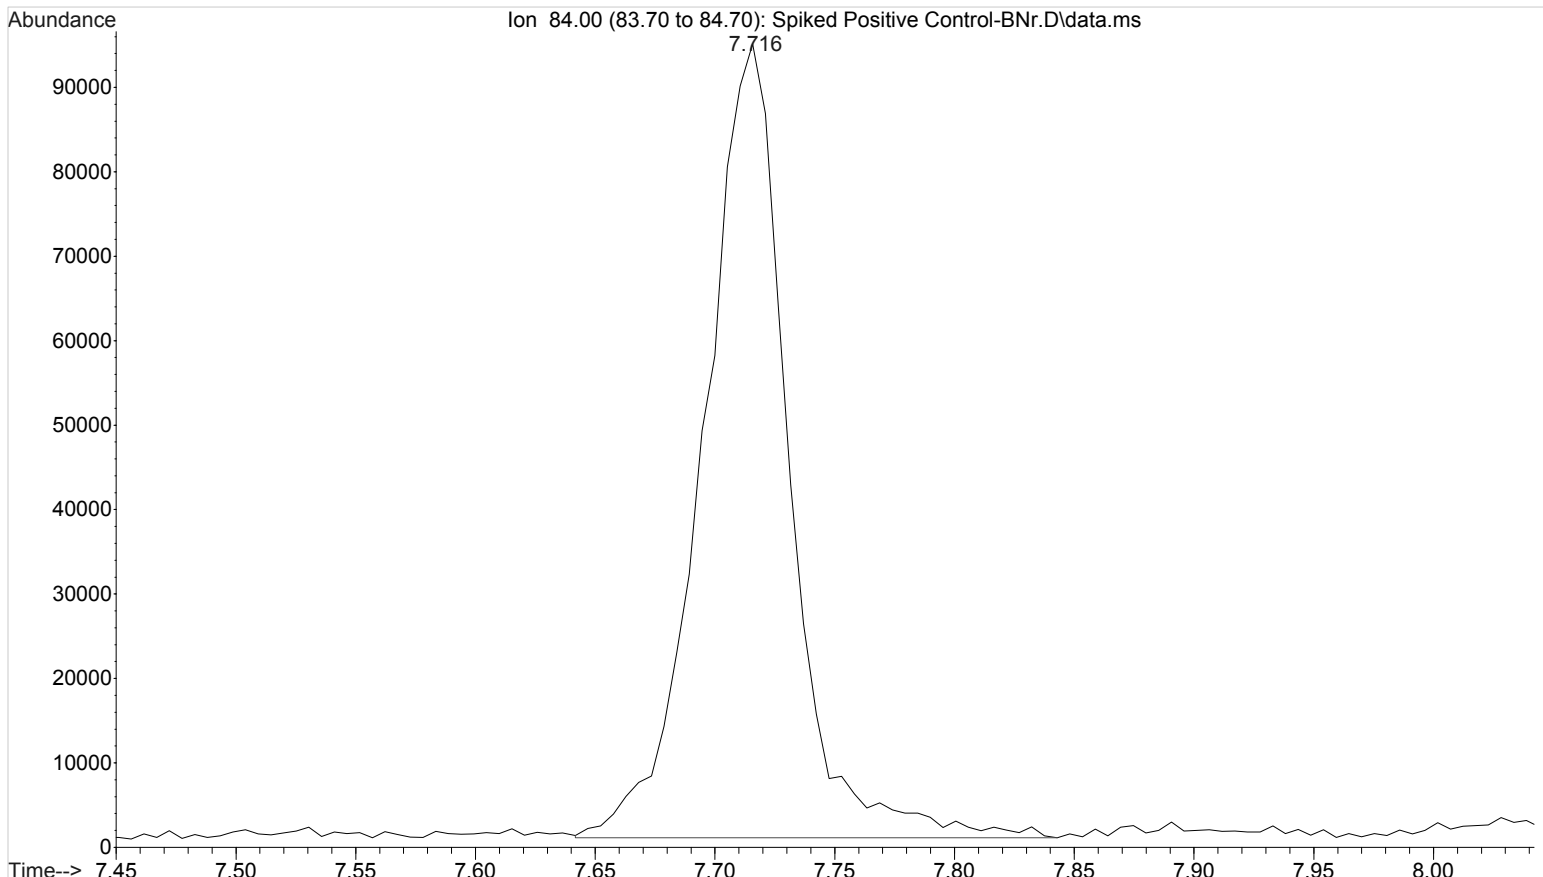


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Spiked Positive Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 15:27 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

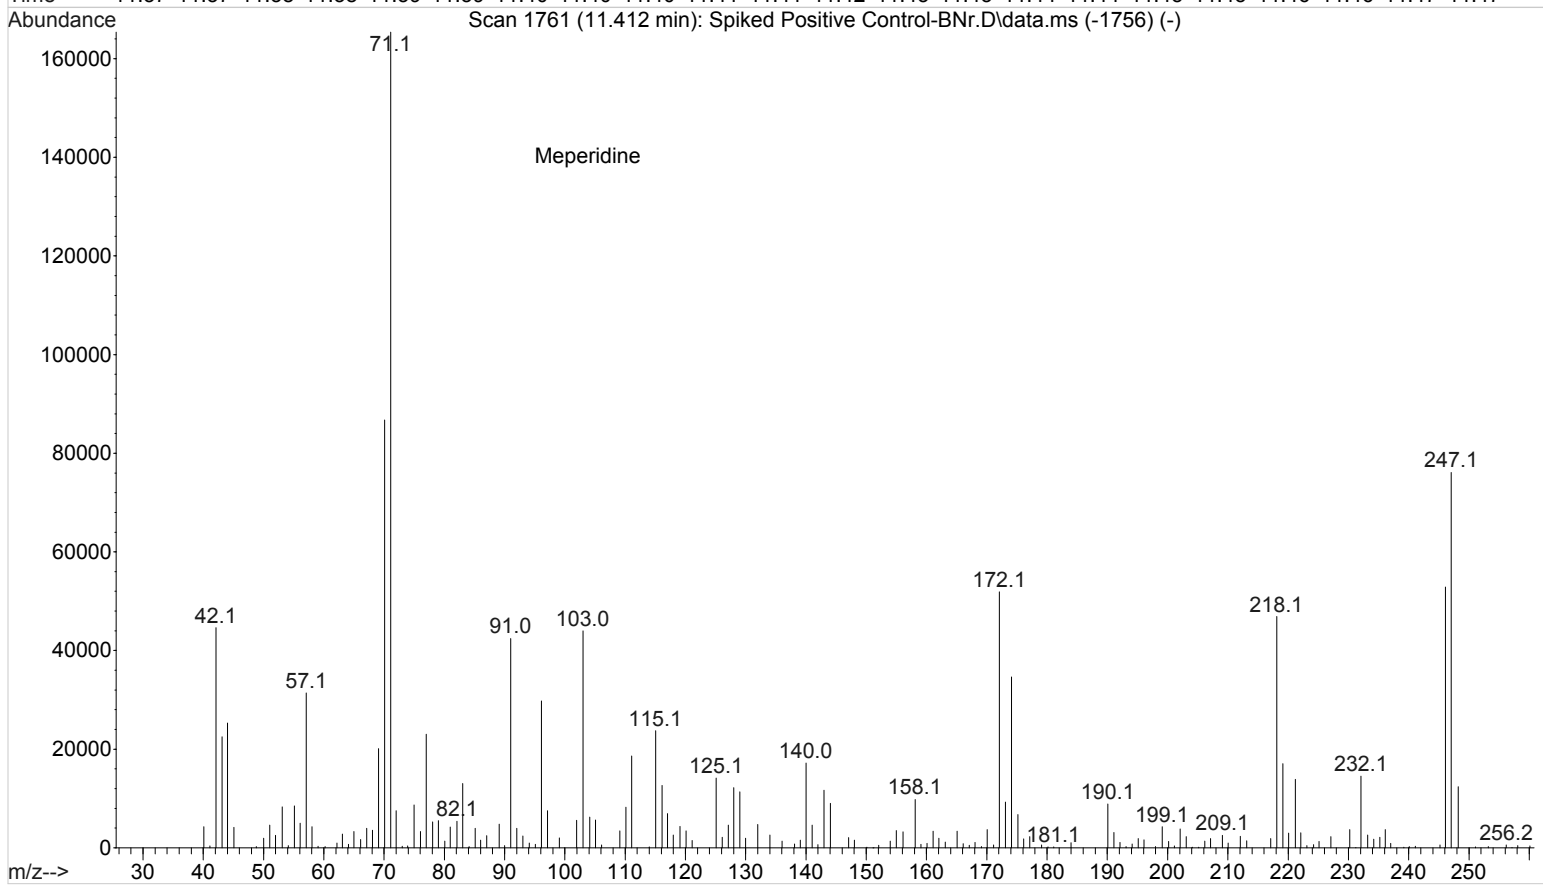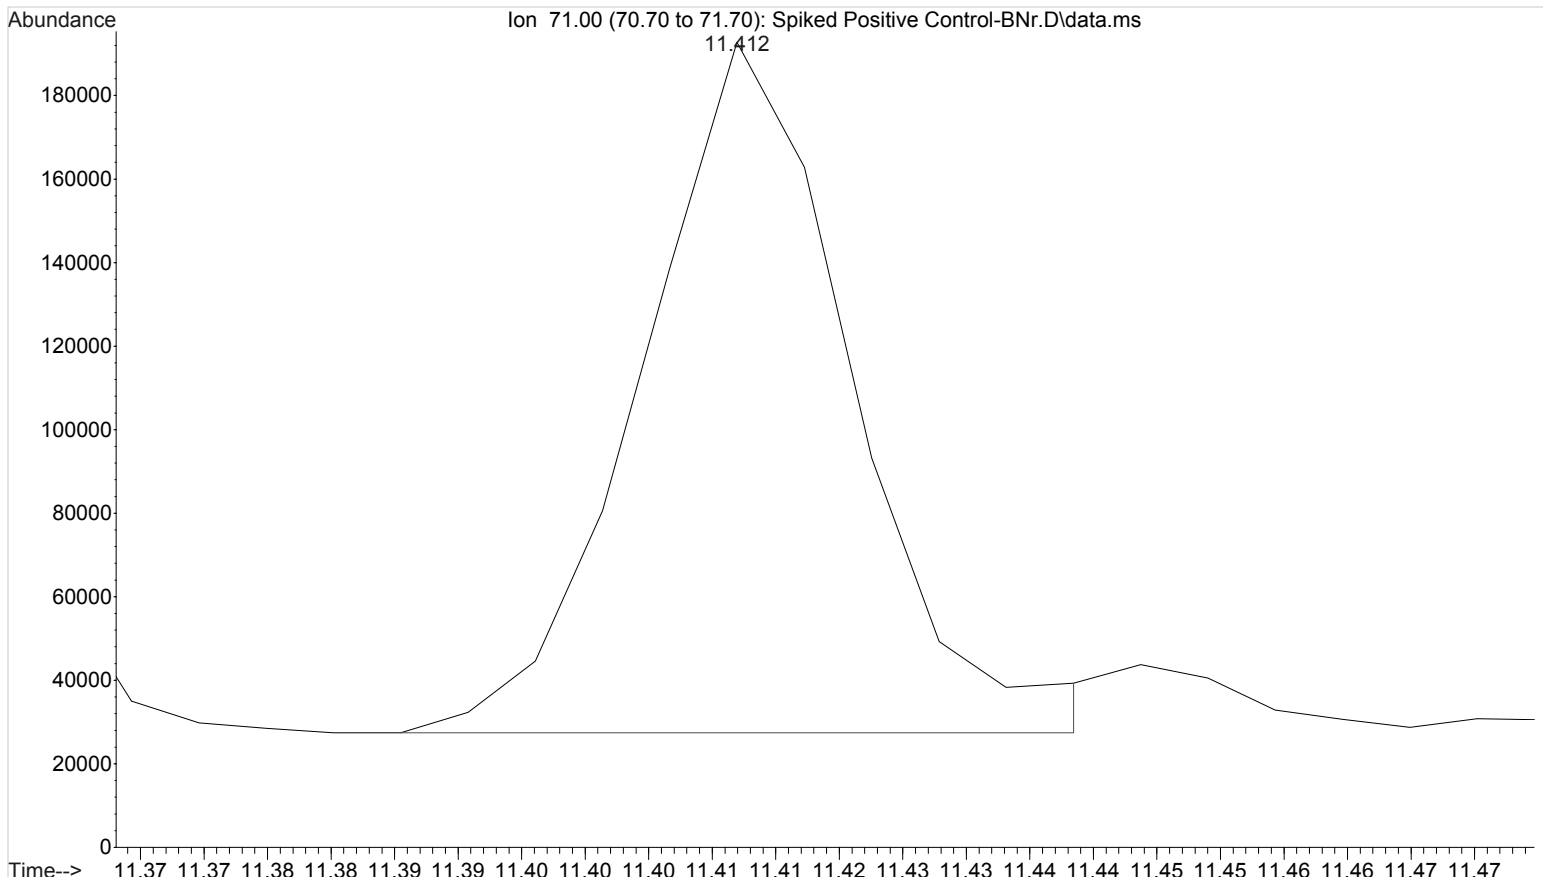





File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Spiked Positive Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 15:27 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

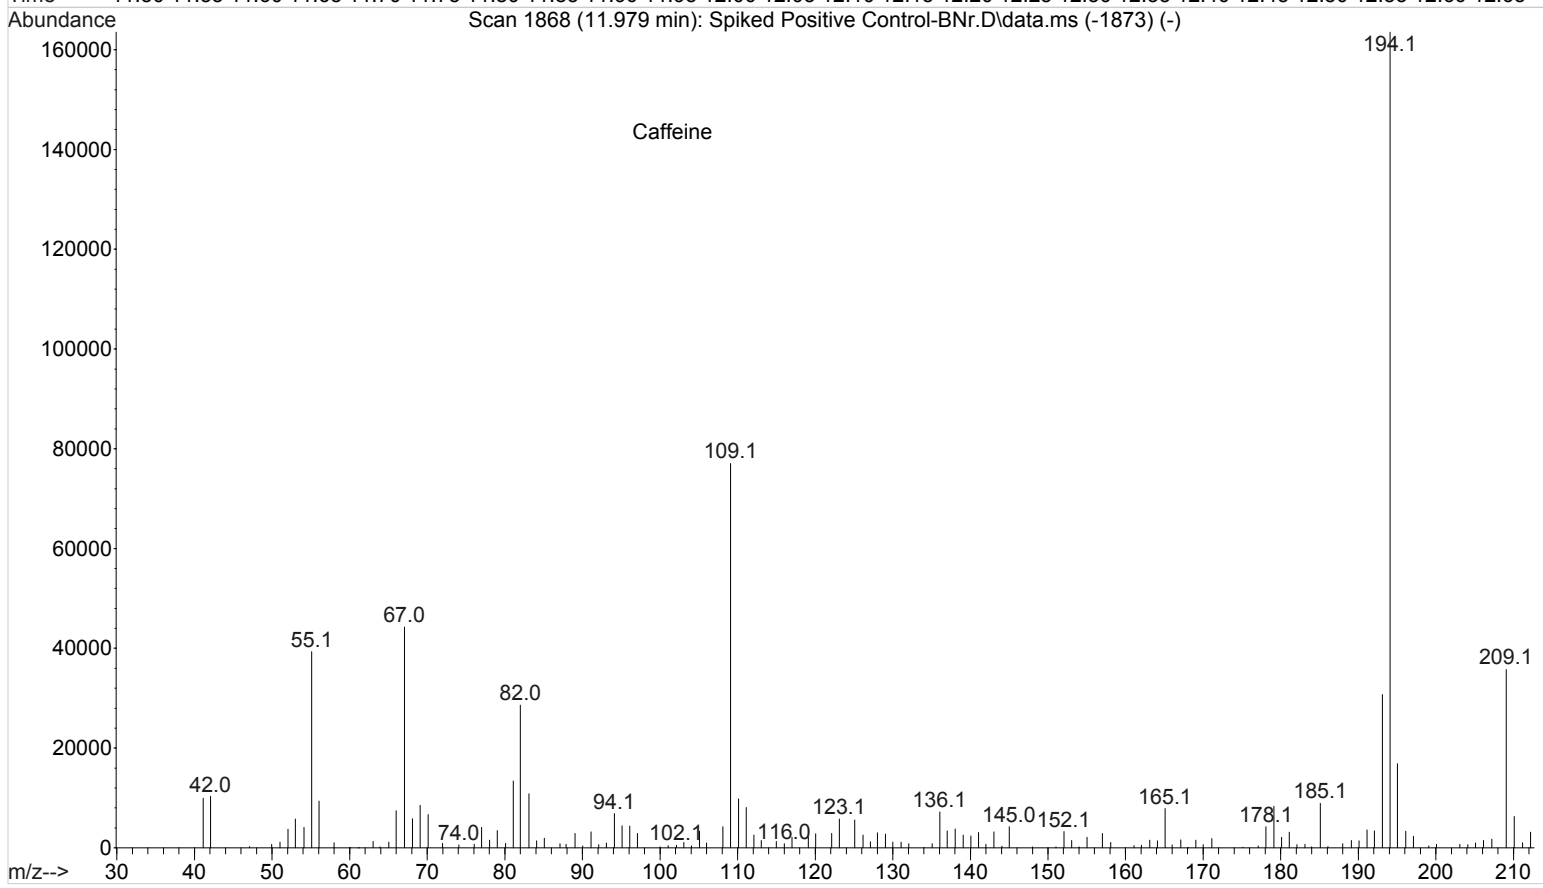
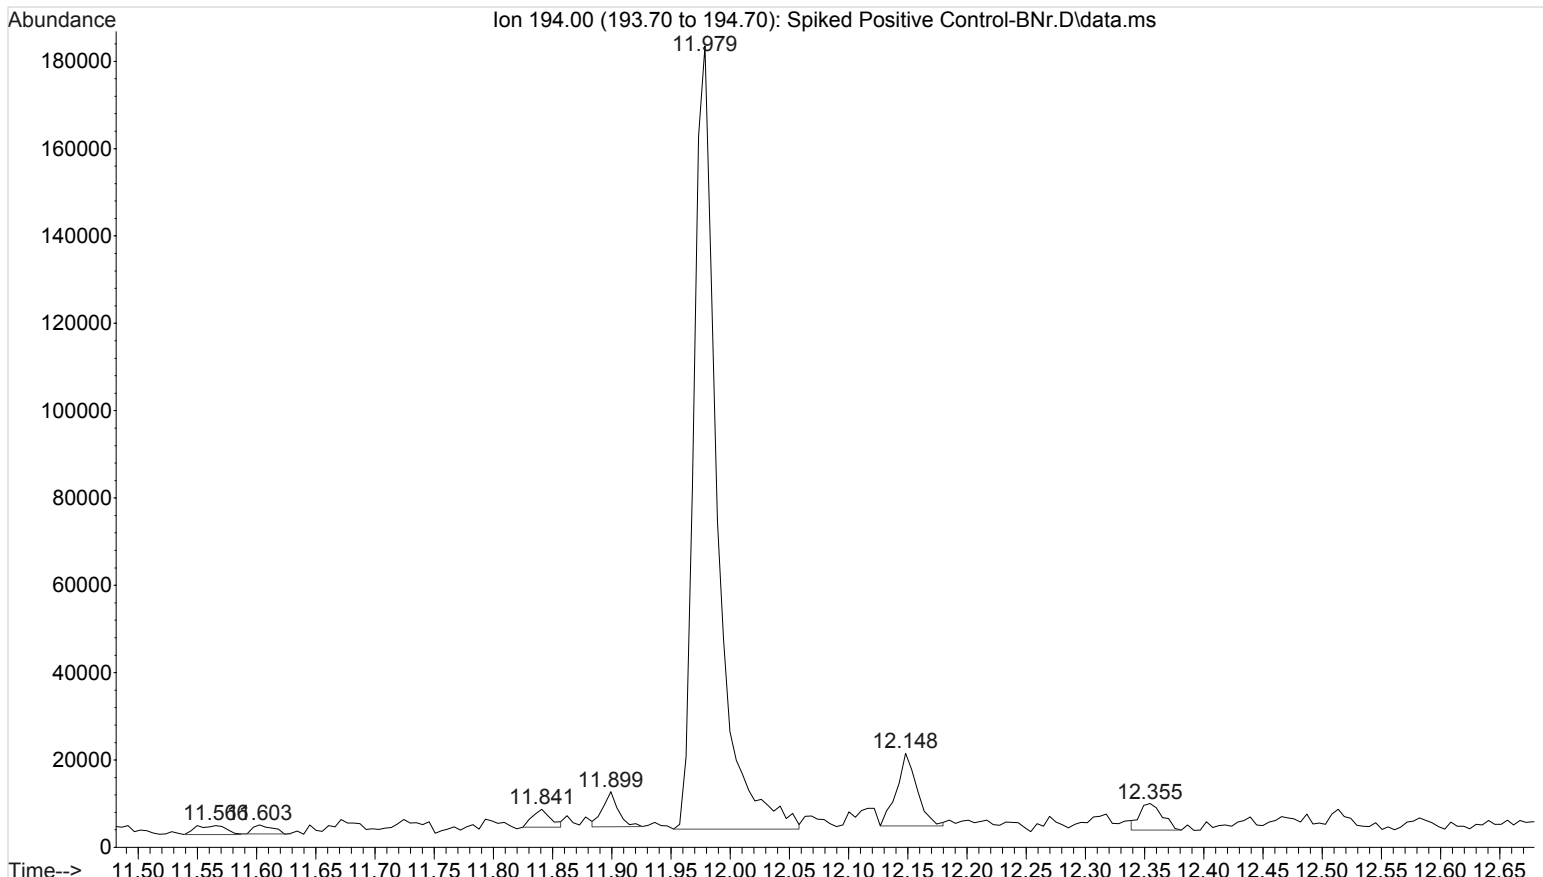


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Spiked Positive Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 15:27 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

9

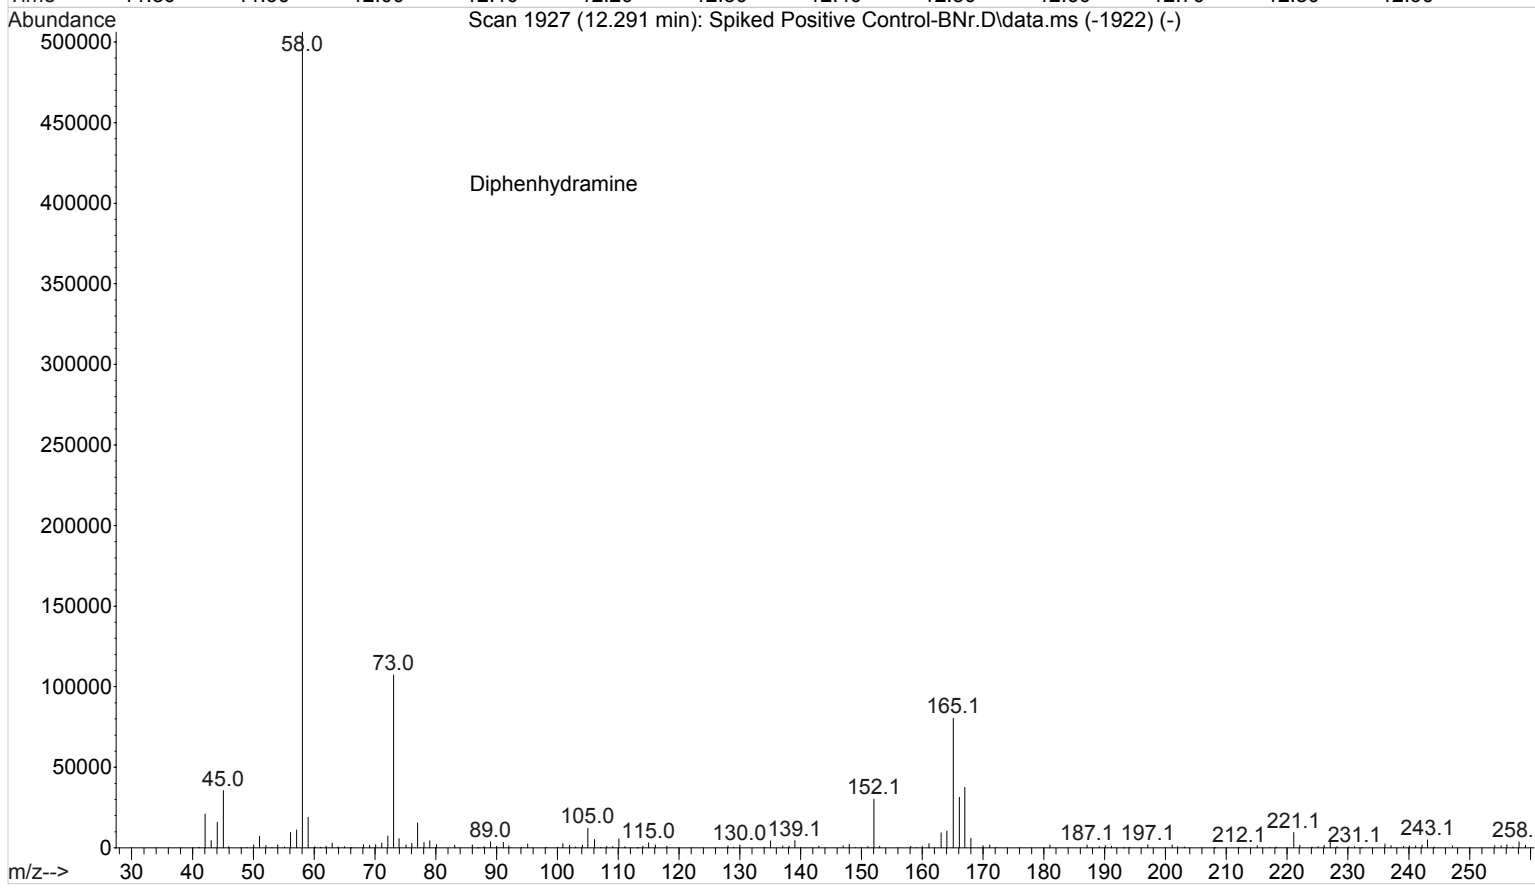
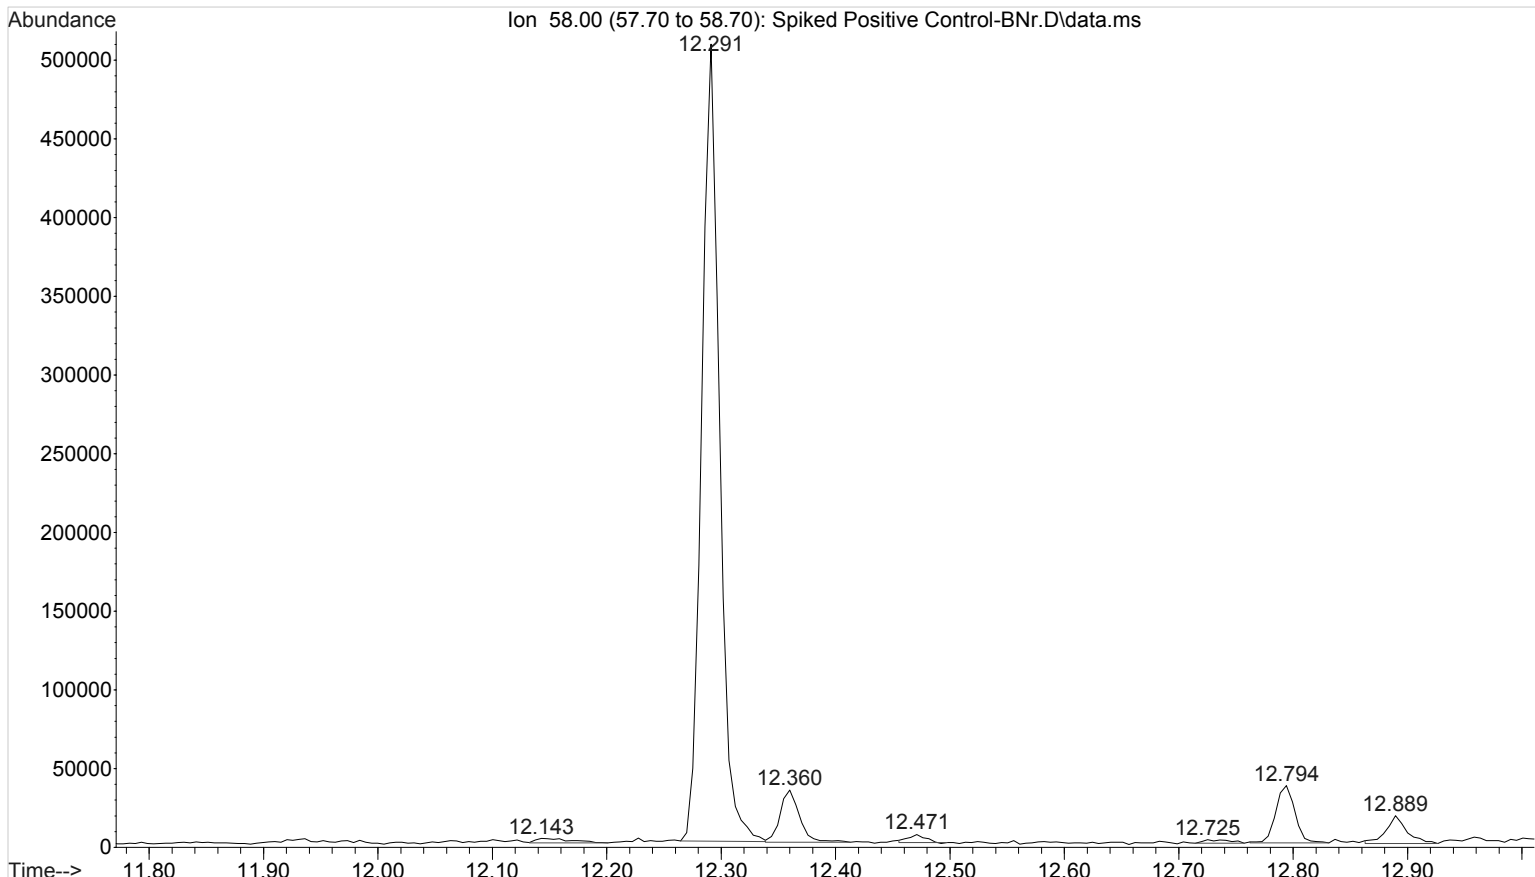


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Spiked Positive Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 15:27 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

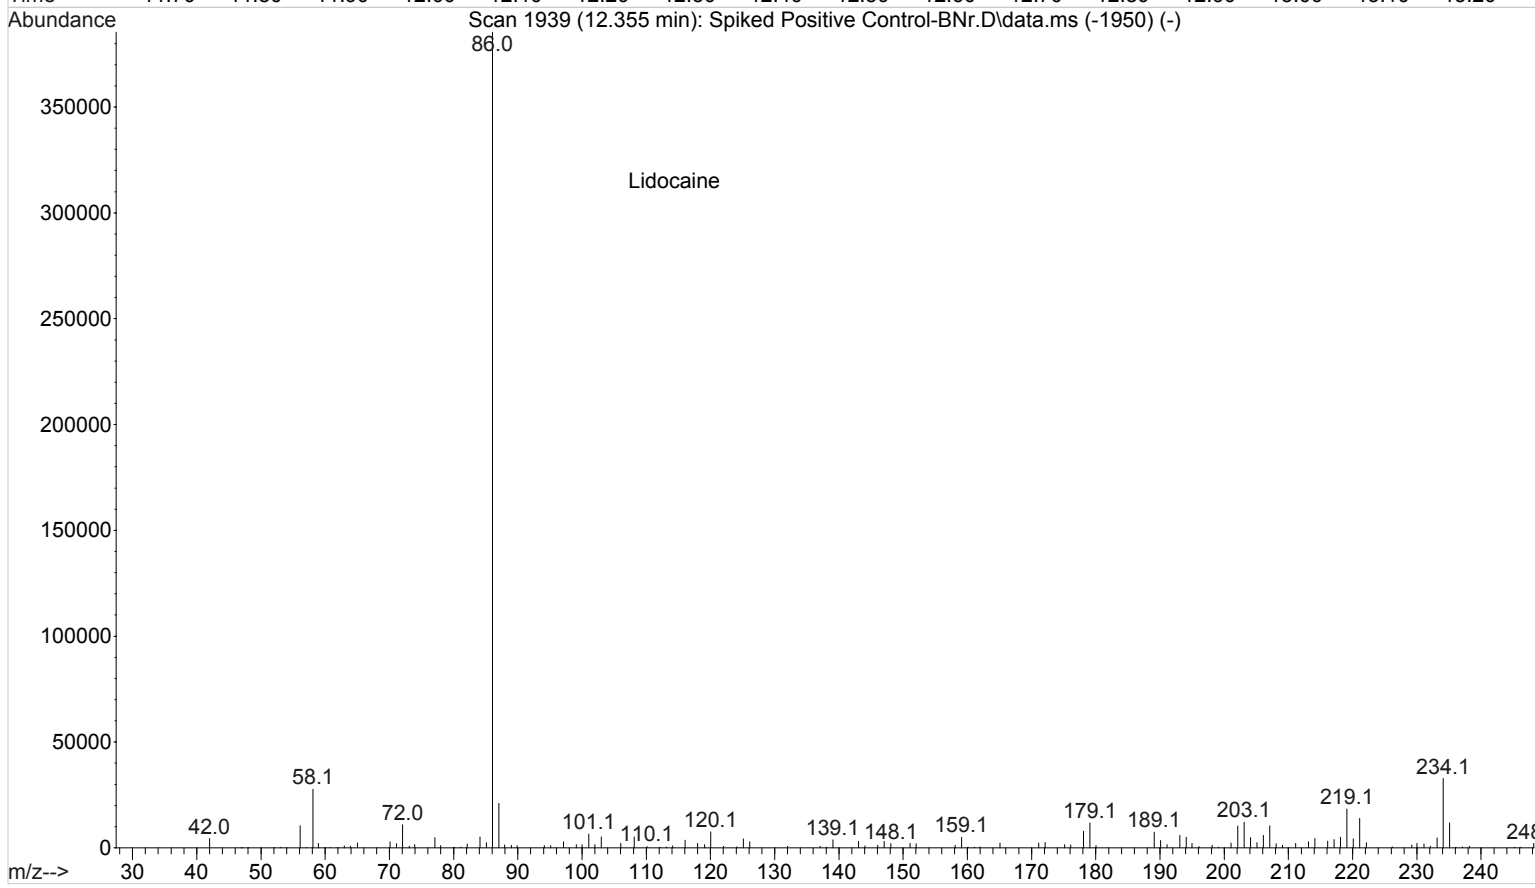
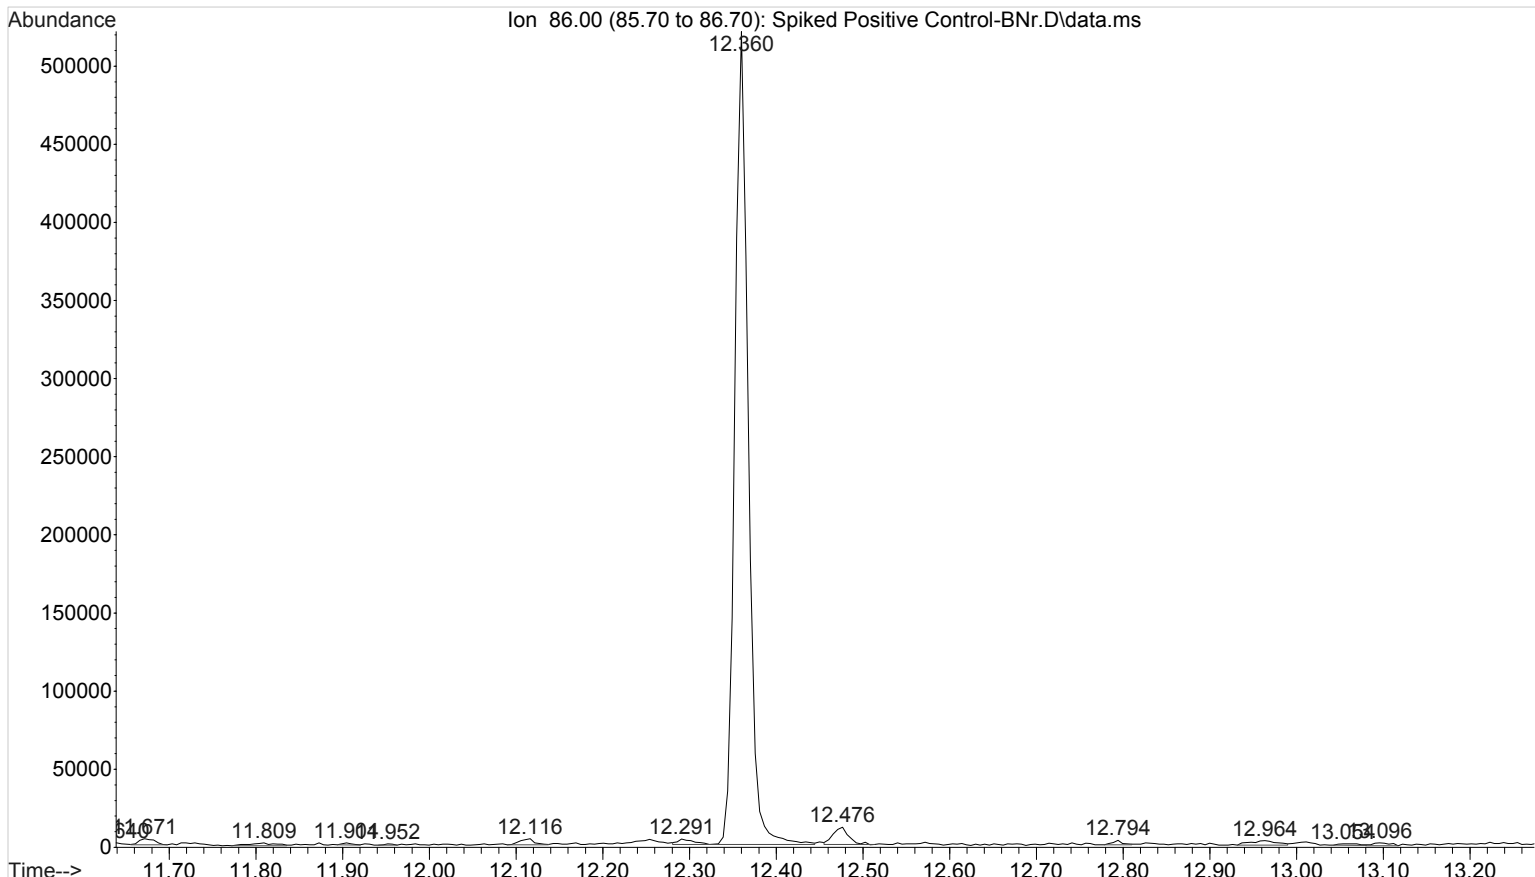


File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Spiked Positive Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 15:27 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215



CS

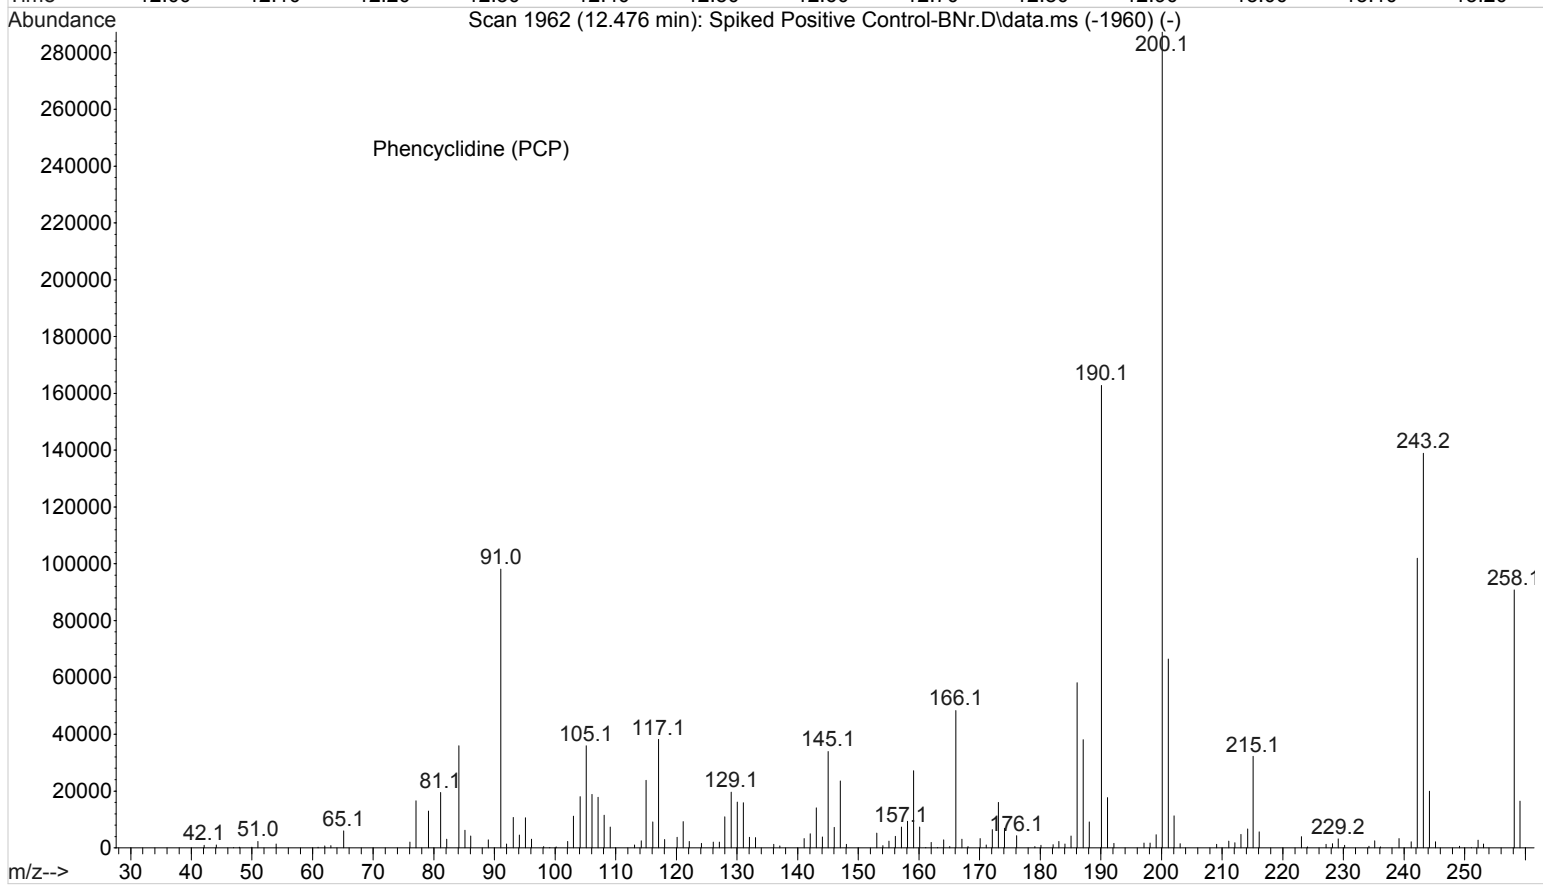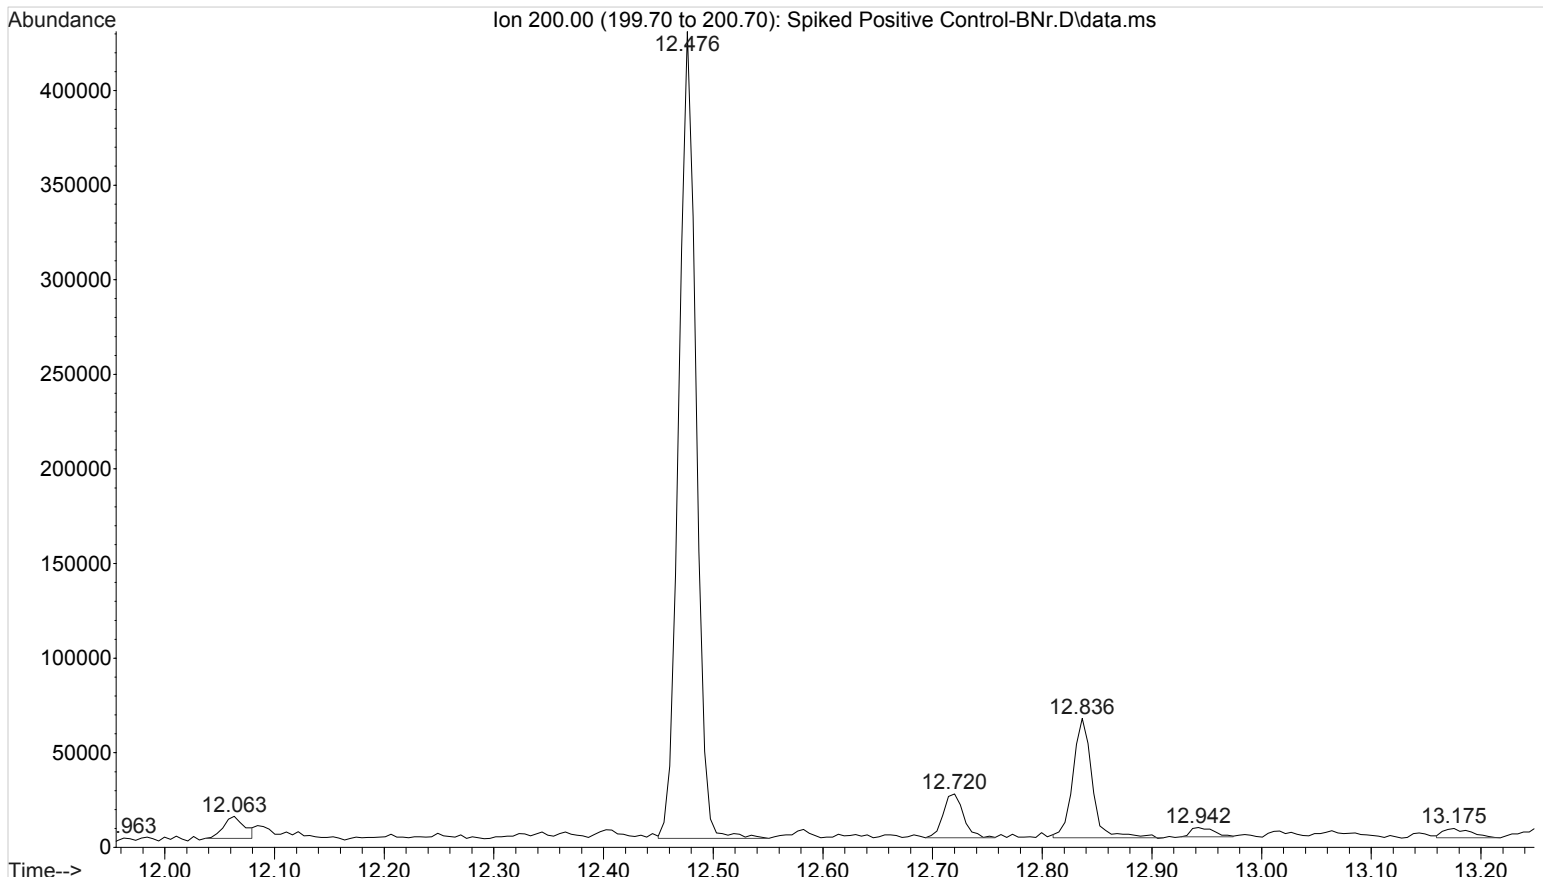



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Spiked Positive Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 15:27 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

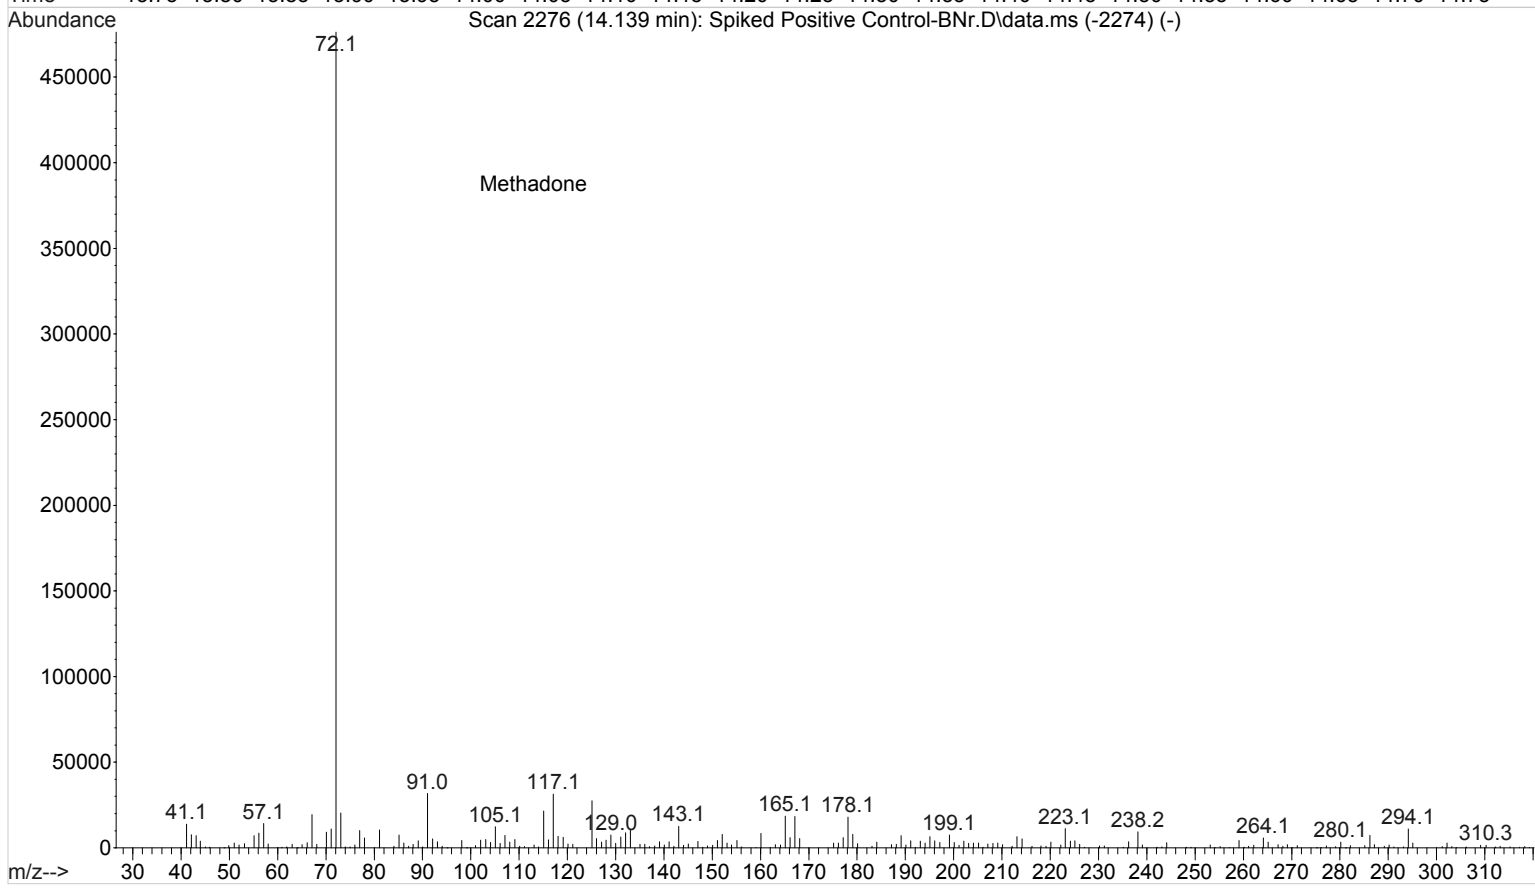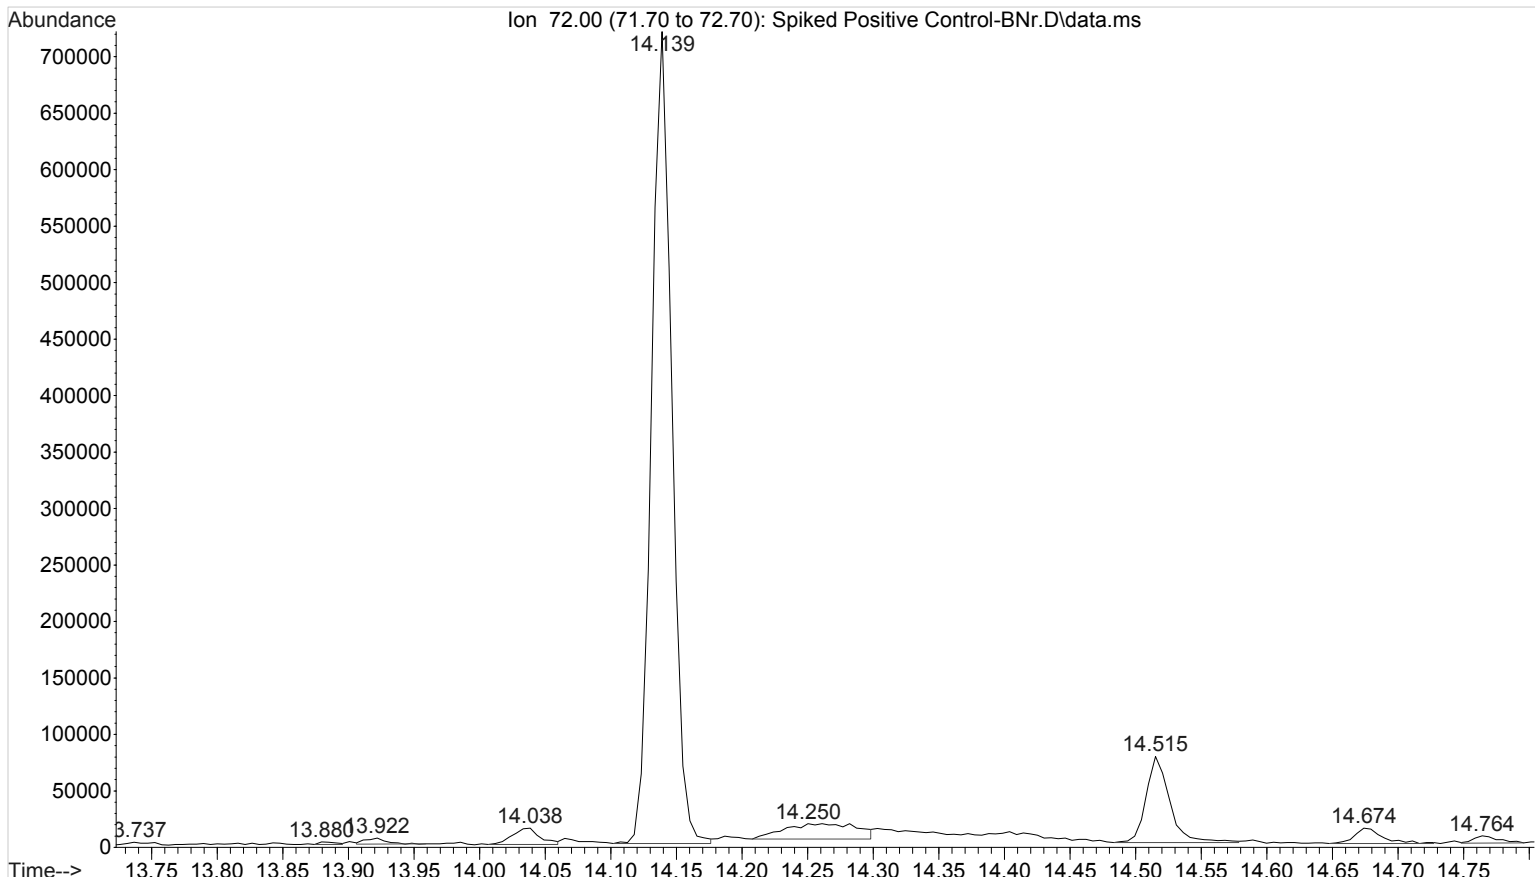



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Spiked Positive Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 15:27 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

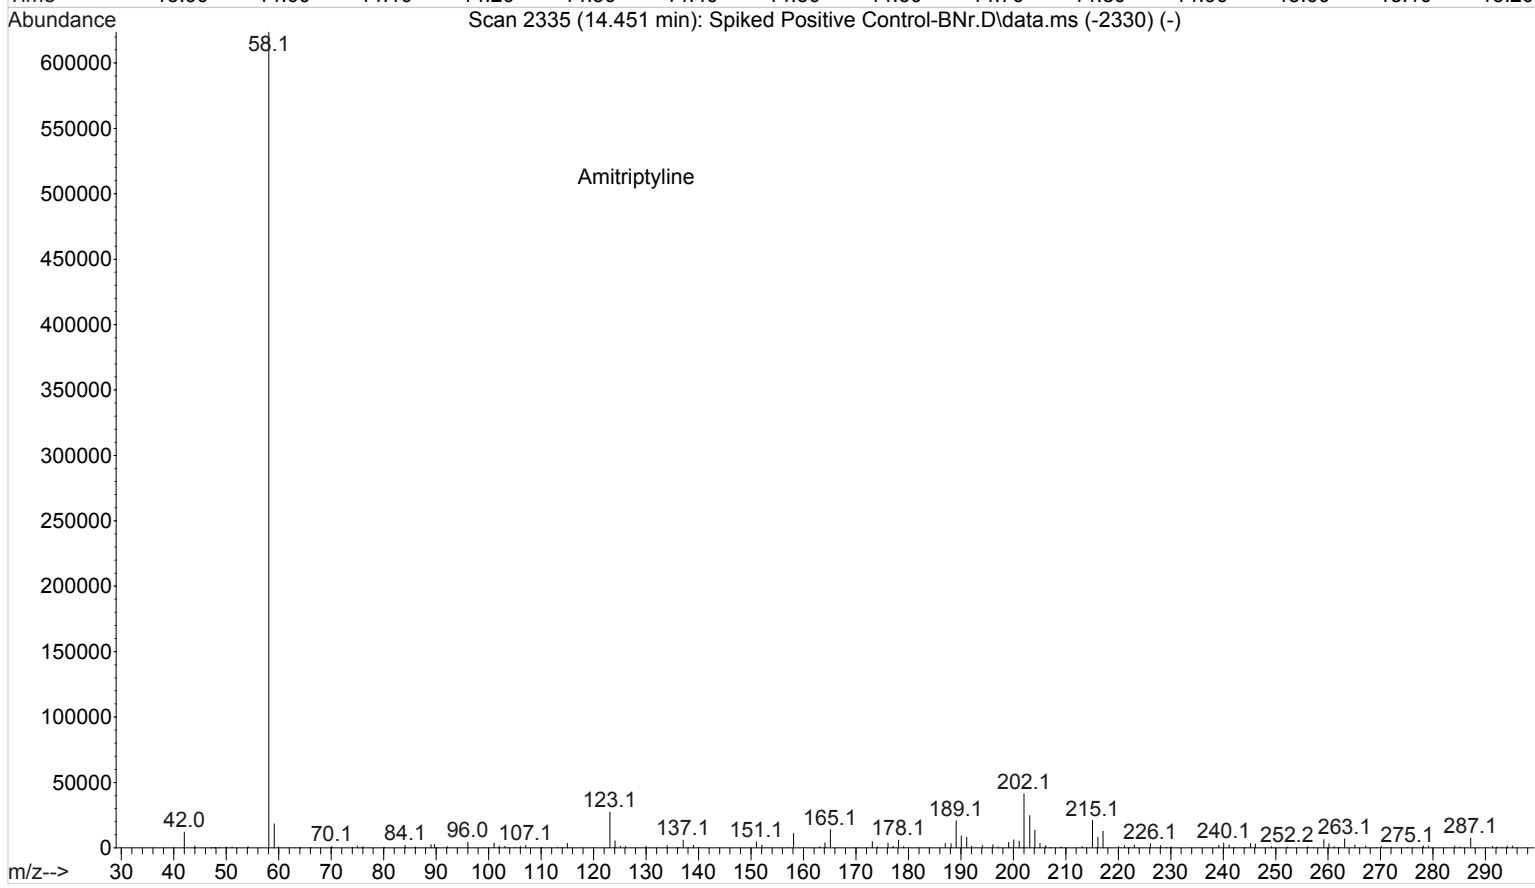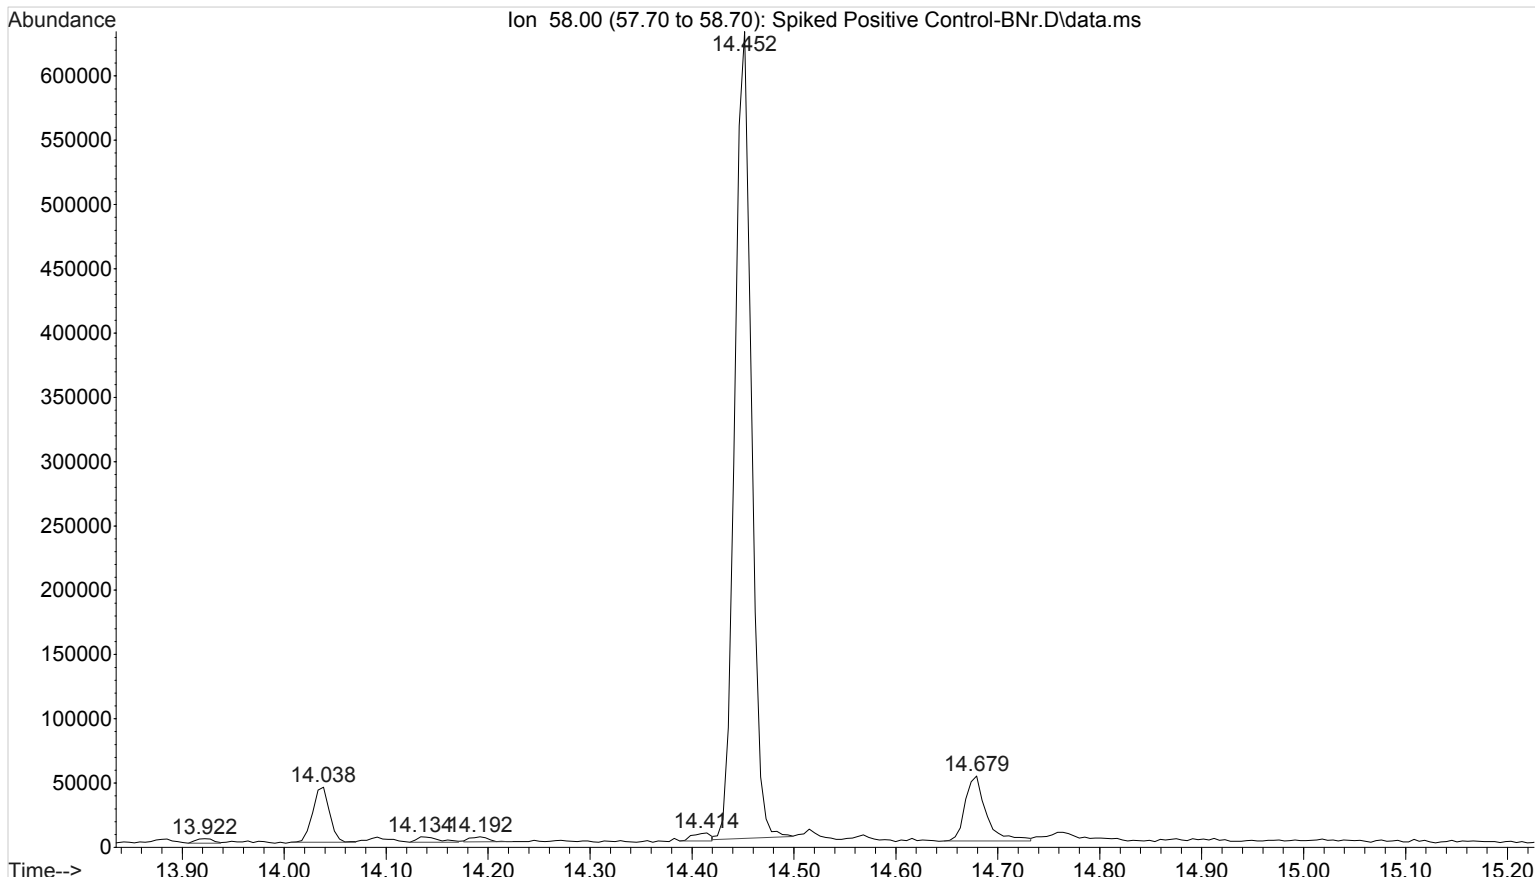

File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Spiked Positive Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 15:27 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

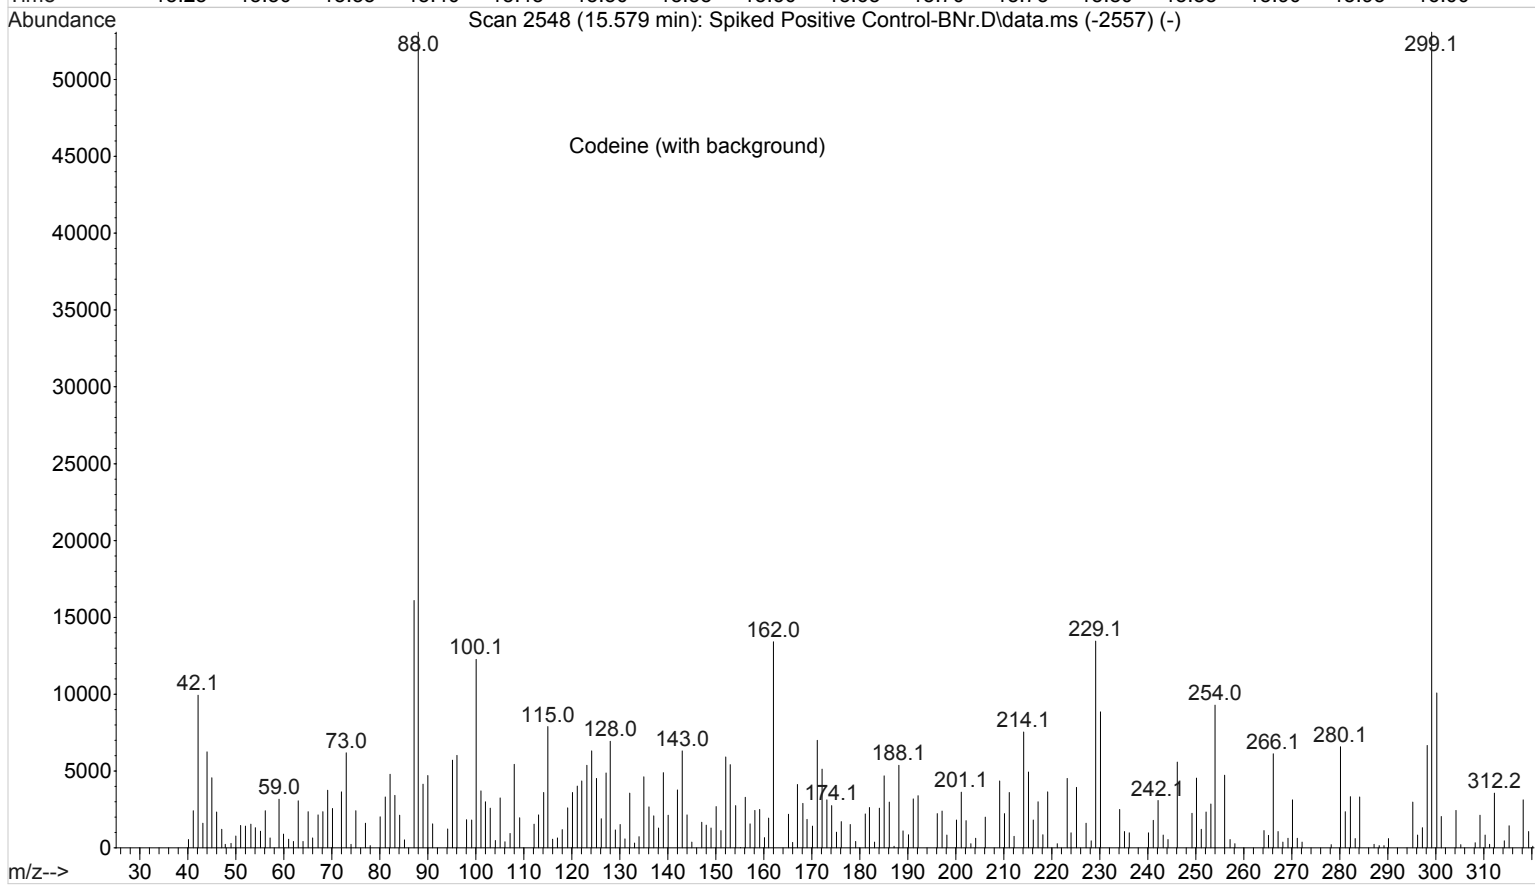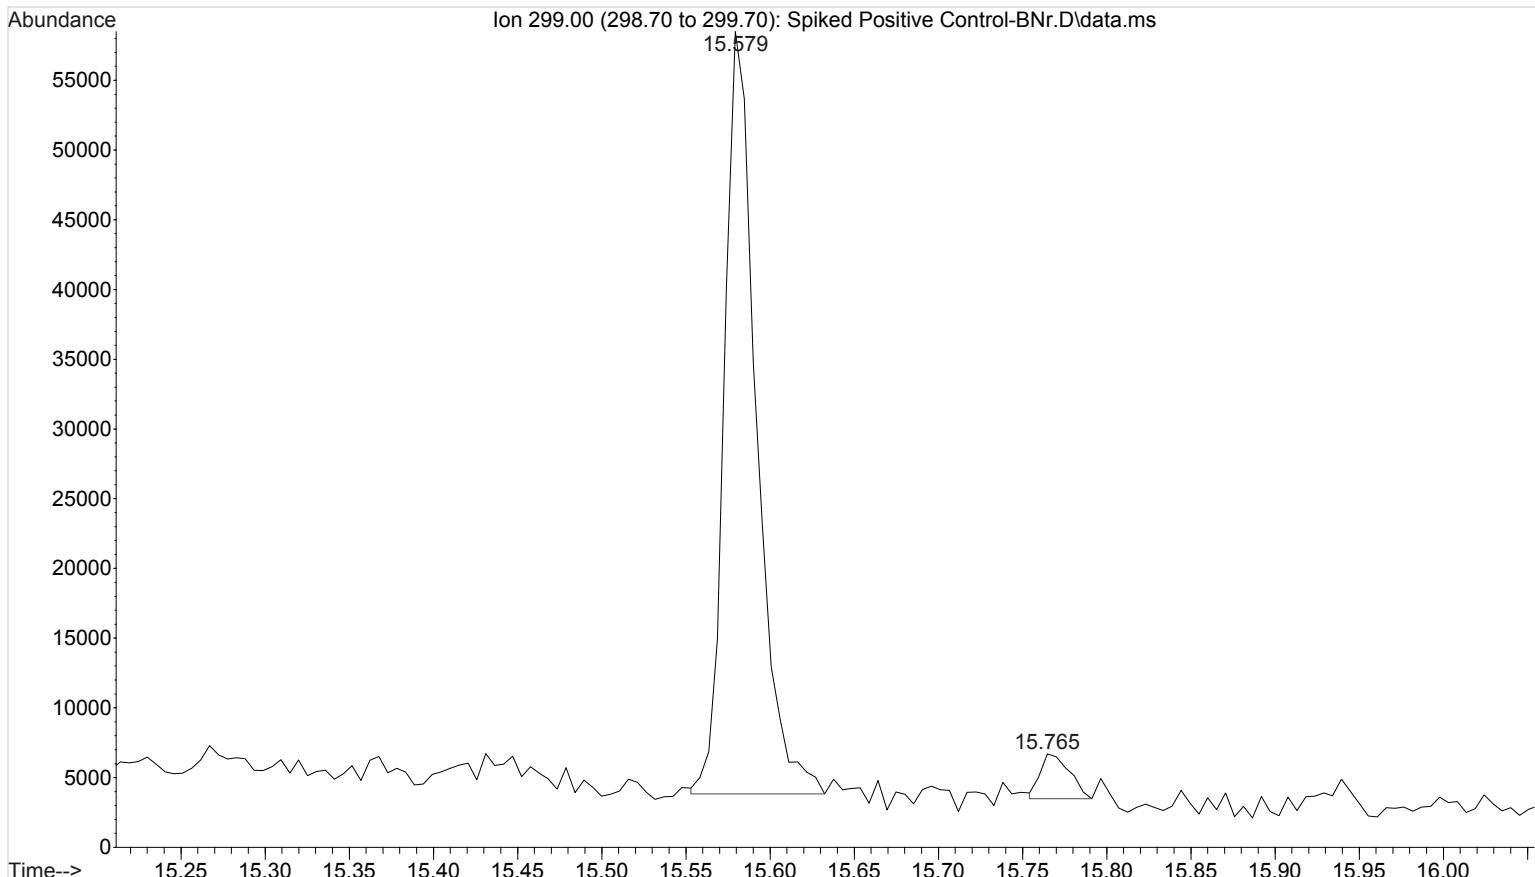

File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \Spiked Positive Control-BNr.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 16 Jun 2016 15:27 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : UTAK B1013 + WS111215

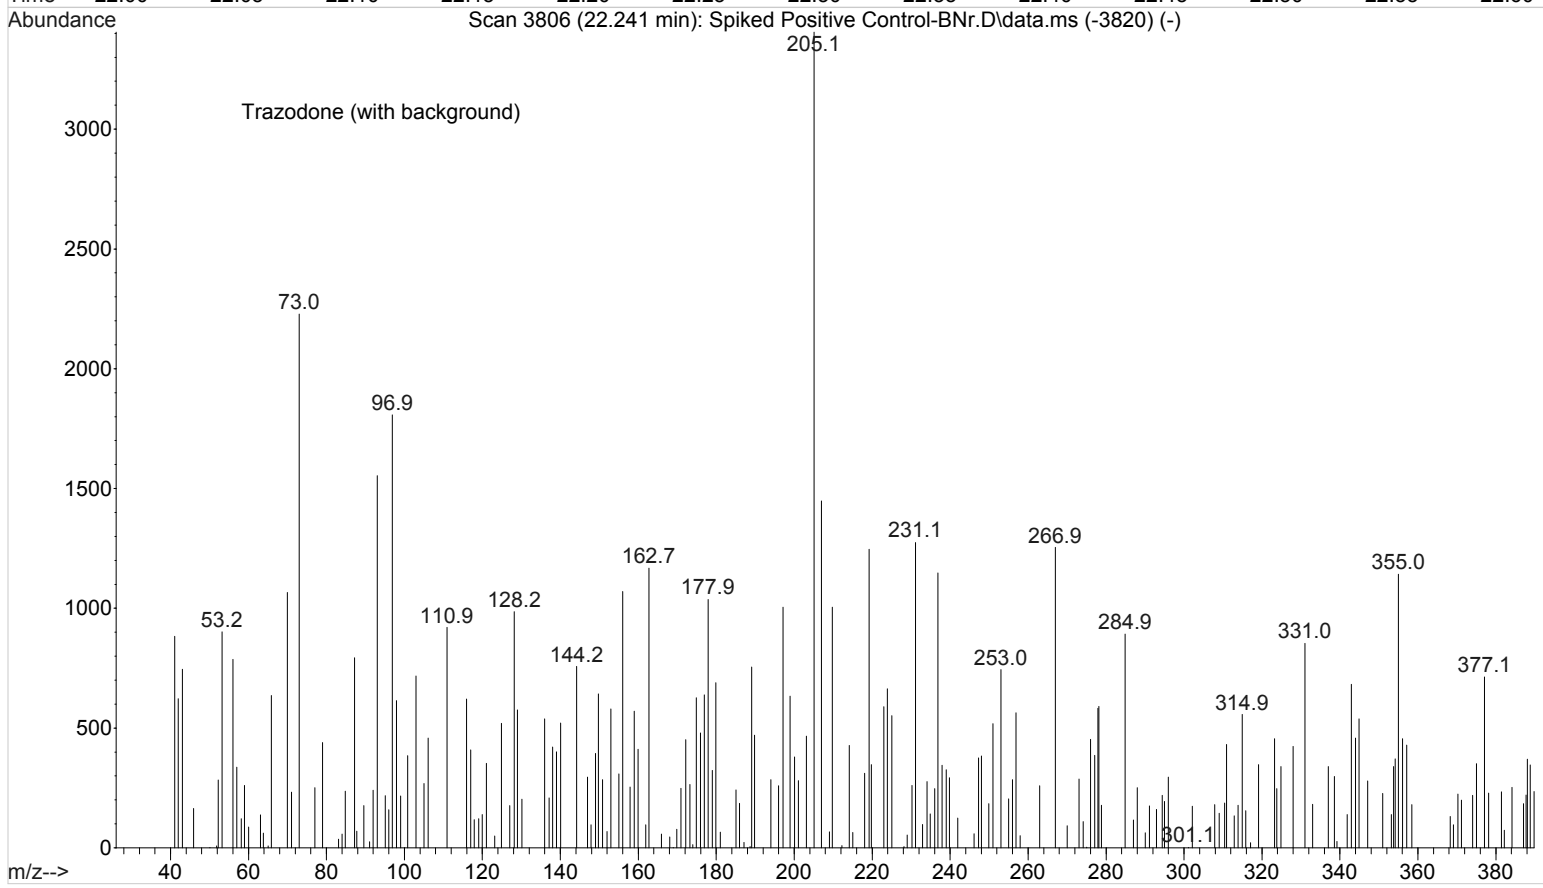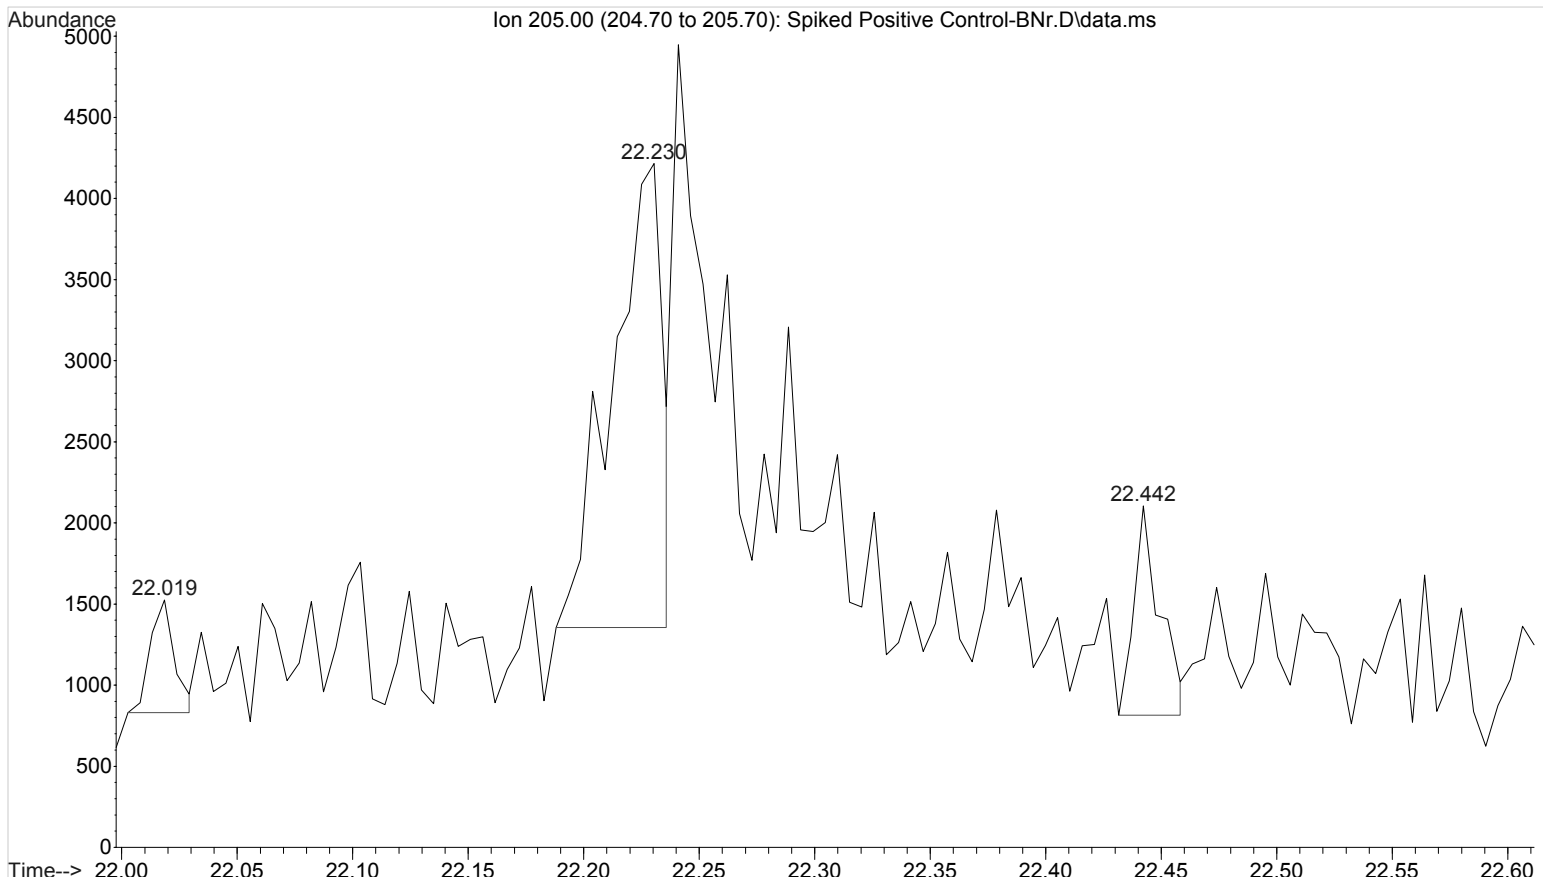



File : I:\Instrument Data\Pocatello\Major Mass Spec\CDS\2016\061616  
... \AFTER.D  
Operator : ISP\datastor  
Instrument : Major Mass Spec  
Acquired : 19 Jun 2016 03:52 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: BLK  
Misc Info : Chloroform

