


1/27/2015



Worklist: 565

<u>LAB CASE</u>	<u>ITEM</u>	<u>TASK ID</u>	<u>DESCRIPTION</u>	
M2014-3411	1	24535	3.6.1 Blood base neutral confirr	
M2014-3561	10	25661	3.6.1 Blood base neutral confirr	
P2014-2751	1	23626	3.6.1 Blood base neutral confirr	
P2014-2782	1	23839	3.6.1 Blood base neutral confirr	
P2014-3002	1	24977	3.6.1 Blood base neutral confirr	
P2014-3004	1	24984	3.6.1 Blood base neutral confirr	
P2014-3080	1	25430	3.6.1 Blood base neutral confirr	
P2014-3104	1	25670	3.6.1 Blood base neutral confirr	
P2014-3105	1	25697	3.6.1 Blood base neutral confirr	
P2014-3110	1	25719	3.6.1 Blood base neutral confirr	
P2014-3113	1	25728	3.6.1 Blood base neutral confirr	
P2014-3115	1	25734	3.6.1 Blood base neutral confirr	
P2015-0001	1	25761	3.6.1 Blood base neutral confirr	
P2015-0015	1	25790	3.6.1 Blood base neutral confirr	
P2015-0023	1	25812	3.6.1 Blood base neutral confirr	
P2015-0056	1	25993	3.6.1 Blood base neutral confirr	
P2015-0073	1	26044	3.6.1 Blood base neutral confirr	
P2015-0119	1	26178	3.6.1 Blood base neutral confirr	
P2015-0122	1	26218	3.6.1 Blood base neutral confirr	
P2015-0150	1	26381	3.6.1 Blood base neutral confirr	
P2015-0154	1	26408	3.6.1 Blood base neutral confirr	
P2015-0155	1	26412	3.6.1 Blood base neutral confirr	
P2015-0156	1	26416	3.6.1 Blood base neutral confirr	

POC-AM36-101232323

Worklist: 565

<u>LAB_CASE</u>	<u>ITEM</u>	<u>TASK_ID</u>	<u>DESCRIPTION</u>
P2015-0157	1	26419	3.6.1 Blood base neutral confir



A handwritten signature in black ink, consisting of a stylized 'P' followed by a loop and a vertical line.

POC_AM 3.6.1_01232015_DND

qr 01/23/15

simulate_sequence.log
Simulate Run Sequence Fri Jan 23 16:02:34 2015

Instrument Name: Major Mass Spec
Sequence File: C:\Users\ISPuser\Desktop\Sequences\DD-BNSB.sequence.xml
Comment: MassHunter sequence
Operator: 5LAB-C01\ISPuser
Data Path: D:\DATA\DND\2015\012315BN\
Method Path: D:\MassHunter\GCMS\1\methods\

Line	Type	Vials	DataFile	Sample Name
Acquisition Method: BNSB120510.M				
1)	Sample	100 ✓	Prerun Solvent Blank	Pre-run Solvent Blank
2)	Sample	1 ✓	Negative Control-BN	Negative Control - ...0
3)	Sample	2 ✓	Spiked Positive Control	Positive Control
4)	Sample	99 ✓	prbLK2	Solvent Blank
Acquisition Method: GBT092509-Delta EMV.M				
5)	Sample	100 ✓	Prerun Solvent Blankr	Pre-run Solvent Blank
6)	Sample	1 ✓	Negative Control-BNr	Negative Control - ...0
7)	Sample	2 ✓	Spiked Positive Control	Positive Control
8)	Sample	99 ✓	prbLK2r	Solvent Blank
Acquisition Method: BNSB120510.M				
9)	Sample	98 ✓	M2014-3411-1-BNBLK	Lab No.: M2014-3411-1
10)	Sample	3 ✓	M2014-3411-1-BN	Lab No.: M2014-3411-1
11)	Sample	97 ✓	M2014-3561-10-BNBLK	Lab No.: M2014-3561-10
12)	Sample	4 ✓	M2014-3561-10-BN	Lab No.: M2014-3561-10
13)	Sample	96 ✓	P2014-2751-1-BNBLK	Lab No.: P2014-2751-1
14)	Sample	5 ✓	P2014-2751-1-BN	Lab No.: P2014-2751-1
15)	Sample	95 ✓	P2014-2782-1-BNBLK	Lab No.: P2014-2782-1
16)	Sample	6 ✓	P2014-2782-1-BN	Lab No.: P2014-2782-1
17)	Sample	93 ✓	P2014-3002-1-BNBLK	Lab No.: P2014-3002-1
18)	Sample	8 ✓	P2014-3002-1-BN	Lab No.: P2014-3002-1
19)	Sample	92 ✓	P2014-3004-1-BNBLK	Lab No.: P2014-3004-1
20)	Sample	9 ✓	P2014-3004-1-BN	Lab No.: P2014-3004-1
21)	Sample	91 ✓	P2014-3080-1-BNBLK	Lab No.: P2014-3080-1
22)	Sample	10 ✓	P2014-3080-1-BN	Lab No.: P2014-3080-1
Acquisition Method: GBT092509-Delta EMV.M				
23)	Sample	98 ✓	M2014-3411-1-BNBLKr	Lab No.: M2014-3411-1
24)	Sample	3 ✓	M2014-3411-1-BNr	Lab No.: M2014-3411-1
25)	Sample	97 ✓	M2014-3561-10-BNBLKr	Lab No.: M2014-3561-10
26)	Sample	4 ✓	M2014-3561-10-BNr	Lab No.: M2014-3561-10
27)	Sample	96 ✓	P2014-2751-1-BNBLKr	Lab No.: P2014-2751-1
28)	Sample	5 ✓	P2014-2751-1-BNr	Lab No.: P2014-2751-1
29)	Sample	95 ✓	P2014-2782-1-BNBLKr	Lab No.: P2014-2782-1
30)	Sample	6 ✓	P2014-2782-1-BNr	Lab No.: P2014-2782-1
31)	Sample	93 ✓	P2014-3002-1-BNBLKr	Lab No.: P2014-3002-1
32)	Sample	8 ✓	P2014-3002-1-BNr	Lab No.: P2014-3002-1
33)	Sample	92 ✓	P2014-3004-1-BNBLKr	Lab No.: P2014-3004-1
34)	Sample	9 ✓	P2014-3004-1-BNr	Lab No.: P2014-3004-1
35)	Sample	91 ✓	P2014-3080-1-BNBLKr	Lab No.: P2014-3080-1
36)	Sample	10 ✓	P2014-3080-1-BNr	Lab No.: P2014-3080-1
Acquisition Method: BNSB120510.M				
37)	Sample	90 ✓	P2014-3104-1-BNBLK	Lab No.: P2014-3104-1
38)	Sample	11 ✓	P2014-3104-1-BN	Lab No.: P2014-3104-1
39)	Sample	89 ✓	P2014-3105-1-BNBLK	Lab No.: P2014-3105-1
40)	Sample	12 ✓	P2014-3105-1-BN	Lab No.: P2014-3105-1
41)	Sample	88 ✓	P2014-3110-1-BNBLK	Lab No.: P2014-3110-1
42)	Sample	13 ✓	P2014-3110-1-BN	Lab No.: P2014-3110-1
43)	Sample	87 ✓	P2014-3113-1-BNBLK	Lab No.: P2014-3113-1
44)	Sample	14 ✓	P2014-3113-1-BN	Lab No.: P2014-3113-1
45)	Sample	86 ✓	P2014-3115-1-BNBLK	Lab No.: P2014-3115-1
46)	Sample	15 ✓	P2014-3115-1-BN	Lab No.: P2014-3115-1

Acquisition Method: GBT092509-Delta EMV.M

QR 01/23/15

simulate_sequence.log			
47) Sample	90	P2014-3104-1-BNBLKr	Lab No.: P2014-3104-1
48) Sample	11	P2014-3104-1-BNr	Lab No.: P2014-3104-1
49) Sample	89	P2014-3105-1-BNBLKr	Lab No.: P2014-3105-1
50) Sample	12	P2014-3105-1-BNr	Lab No.: P2014-3105-1
51) Sample	88	P2014-3110-1-BNBLKr	Lab No.: P2014-3110-1
52) Sample	13	P2014-3110-1-BNr	Lab No.: P2014-3110-1
53) Sample	87	P2014-3113-1-BNBLKr	Lab No.: P2014-3113-1
54) Sample	14	P2014-3113-1-BNr	Lab No.: P2014-3113-1
55) Sample	86	P2014-3115-1-BNBLKr	Lab No.: P2014-3115-1
56) Sample	15	P2014-3115-1-BNr	Lab No.: P2014-3115-1

Acquisition Method: BNSB120510.M

57) Sample	85	P2015-0001-1-BNBLK	Lab No.: P2015-0001-1
58) Sample	16	P2015-0001-1-BN	Lab No.: P2015-0001-1
59) Sample	84	P2015-0015-1-BNBLK	Lab No.: P2015-0015-1
60) Sample	17	P2015-0015-1-BN	Lab No.: P2015-0015-1
61) Sample	83	P2015-0023-1-BNBLK	Lab No.: P2015-0023-1
62) Sample	18	P2015-0023-1-BN	Lab No.: P2015-0023-1
63) Sample	82	P2015-0056-1-BNBLK	Lab No.: P2015-0056-1
64) Sample	19	P2015-0056-1-BN	Lab No.: P2015-0056-1
65) Sample	81	P2015-0073-1-BNBLK	Lab No.: P2015-0073-1
66) Sample	20	P2015-0073-1-BN	Lab No.: P2015-0073-1

Acquisition Method: GBT092509-Delta EMV.M

67) Sample	85	P2015-0001-1-BNBLKr	Lab No.: P2015-0001-1
68) Sample	16	P2015-0001-1-BNr	Lab No.: P2015-0001-1
69) Sample	84	P2015-0015-1-BNBLKr	Lab No.: P2015-0015-1
70) Sample	17	P2015-0015-1-BNr	Lab No.: P2015-0015-1
71) Sample	83	P2015-0023-1-BNBLKr	Lab No.: P2015-0023-1
72) Sample	18	P2015-0023-1-BNr	Lab No.: P2015-0023-1
73) Sample	82	P2015-0056-1-BNBLKr	Lab No.: P2015-0056-1
74) Sample	19	P2015-0056-1-BNr	Lab No.: P2015-0056-1
75) Sample	81	P2015-0073-1-BNBLKr	Lab No.: P2015-0073-1
76) Sample	20	P2015-0073-1-BNr	Lab No.: P2015-0073-1

Acquisition Method: BNSB120510.M

77) Sample	80	P2015-0119-1-BNBLK	Lab No.: P2015-0119-1
78) Sample	21	P2015-0119-1-BN	Lab No.: P2015-0119-1
79) Sample	79	P2015-0122-1-BNBLK	Lab No.: P2015-0122-1
80) Sample	22	P2015-0122-1-BN	Lab No.: P2015-0122-1
81) Sample	78	P2015-0150-1-BNBLK	Lab No.: P2015-0150-1
82) Sample	23	P2015-0150-1-BN	Lab No.: P2015-0150-1
83) Sample	77	P2015-0154-1-BNBLK	Lab No.: P2015-0154-1
84) Sample	24	P2015-0154-1-BN	Lab No.: P2015-0154-1
85) Sample	76	P2015-0155-1-BNBLK	Lab No.: P2015-0155-1
86) Sample	25	P2015-0155-1-BN	Lab No.: P2015-0155-1

Acquisition Method: GBT092509-Delta EMV.M

87) Sample	80	P2015-0119-1-BNBLKr	Lab No.: P2015-0119-1
88) Sample	21	P2015-0119-1-BNr	Lab No.: P2015-0119-1
89) Sample	79	P2015-0122-1-BNBLKr	Lab No.: P2015-0122-1
90) Sample	22	P2015-0122-1-BNr	Lab No.: P2015-0122-1
91) Sample	78	P2015-0150-1-BNBLKr	Lab No.: P2015-0150-1
92) Sample	23	P2015-0150-1-BNr	Lab No.: P2015-0150-1
93) Sample	77	P2015-0154-1-BNBLKr	Lab No.: P2015-0154-1
94) Sample	24	P2015-0154-1-BNr	Lab No.: P2015-0154-1
95) Sample	76	P2015-0155-1-BNBLKr	Lab No.: P2015-0155-1
96) Sample	25	P2015-0155-1-BNr	Lab No.: P2015-0155-1

Acquisition Method: BNSB120510.M

97) Sample	75	P2015-0156-1-BNBLK	Lab No.: P2015-0156-1
98) Sample	26	P2015-0156-1-BN	Lab No.: P2015-0156-1
99) Sample	74	P2015-0157-1-BNBLK	Lab No.: P2015-0157-1
100) Sample	27	P2015-0157-1-BN	Lab No.: P2015-0157-1

Acquisition Method: GBT092509-Delta EMV.M

101) Sample	75	P2015-0156-1-BNBLKr	Lab No.: P2015-0156-1
102) Sample	26	P2015-0156-1-BNr	Lab No.: P2015-0156-1

01/23/15

103) Sample 74 / simulate_sequence.log
104) Sample 27 / P2015-0157-1-BNBLKr
P2015-0157-1-BNr

Lab No.: P2015-0157-1
Lab No.: P2015-0157-1

Acquisition Method: BNSB120510.M
105) Sample 73 / POSTBLK

BLK

Acquisition Method: GBT092509-Delta EMV.M
106) Sample 72 / AFTER
megabytes Needed: 1715 Space on drive D: 320265
Sequence Verification Done!

BLK

POC_AM 3.6.1_01232015_DVD

Analytical Method 3.6.1 & 3.6.7 QA Check List

Run Start Date: 01/23/15

Analyst: DND

(Short GC/MS temperature program)

Positive Control Compound List

- Methamphetamine
- Nicotine
- Meperidine
- Caffeine
- Diphenhydramine
- Lidocaine
- PCP
- Methadone
- Amitriptyline
- Codeine
- (Trazodone)



Internal Standards

- Benzphetamine
- Papaverine


Optional back extraction **not** performed.
Samples reconstituted in methanol.





File :C:\gcms\1\data\Blood\012315BN\Prerun Solvent Blank.D
Operator : 5LAB-C01\ISPuser
Acquired : 23 Jan 2015 16:49 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Pre-run Solvent Blank
Misc Info : Chloroform
Vial Number: 100

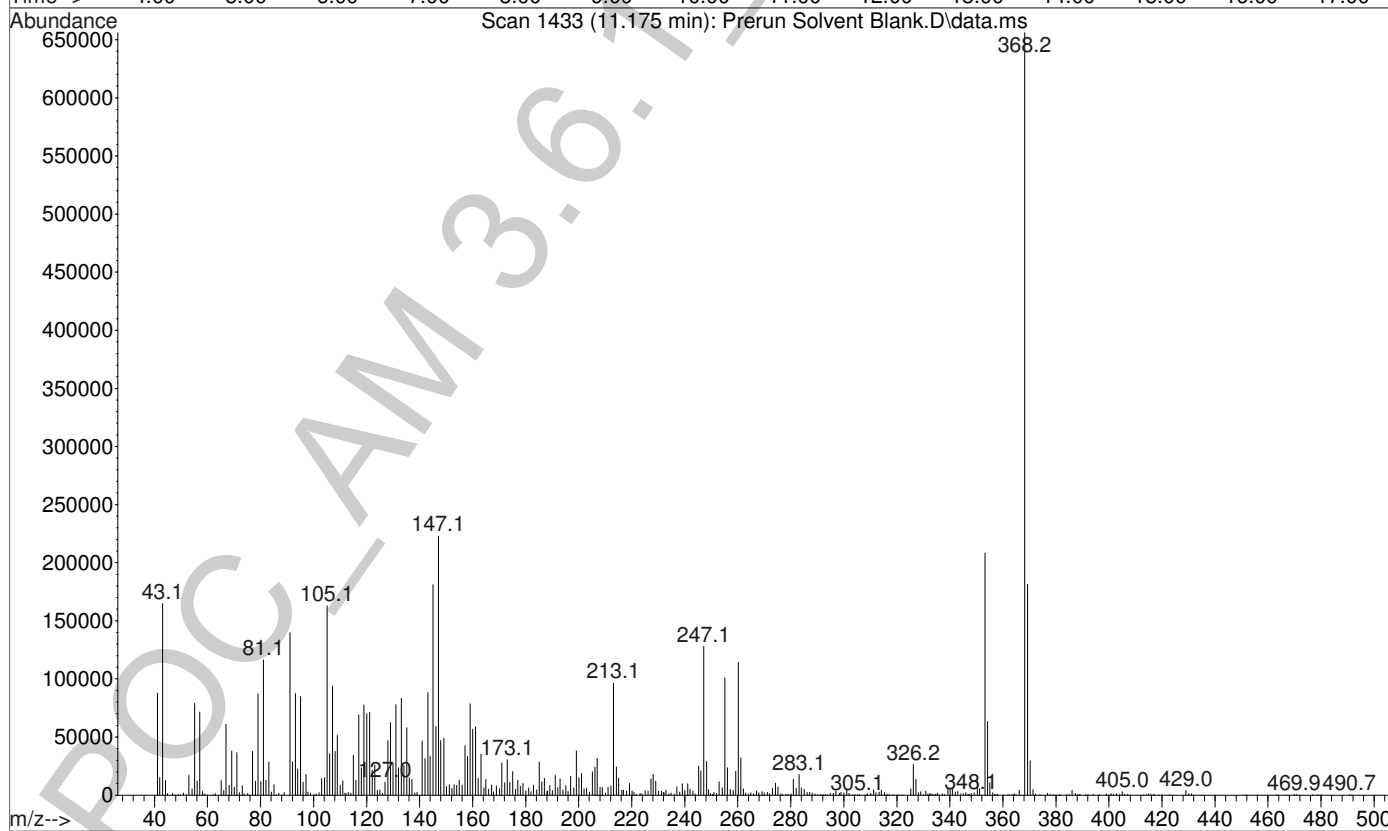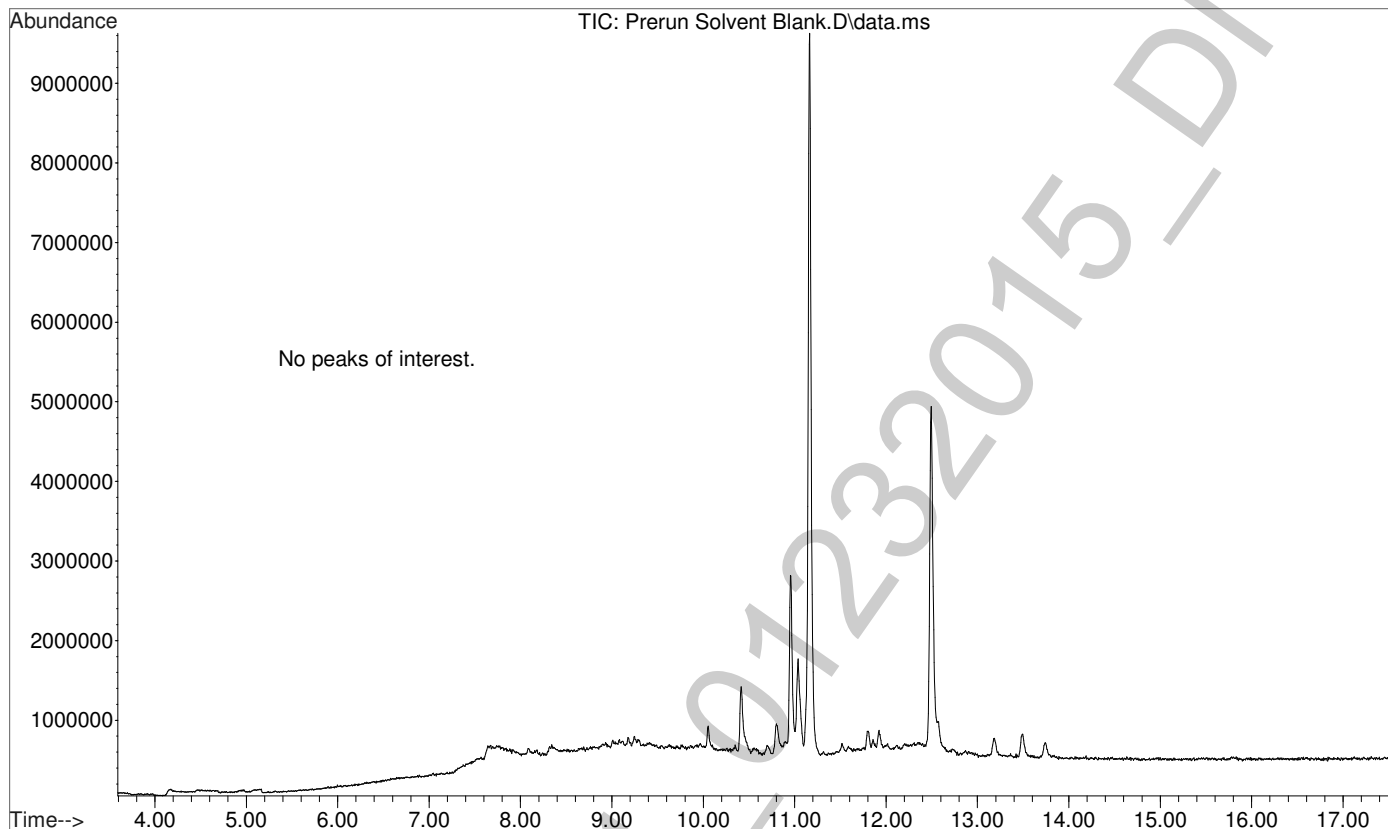



File :C:\gcms\1\data\Blood\012315BN\Negative Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 23 Jan 2015 17:12 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0130
Misc Info : Analytical Method 3.6.1
Vial Number: 1

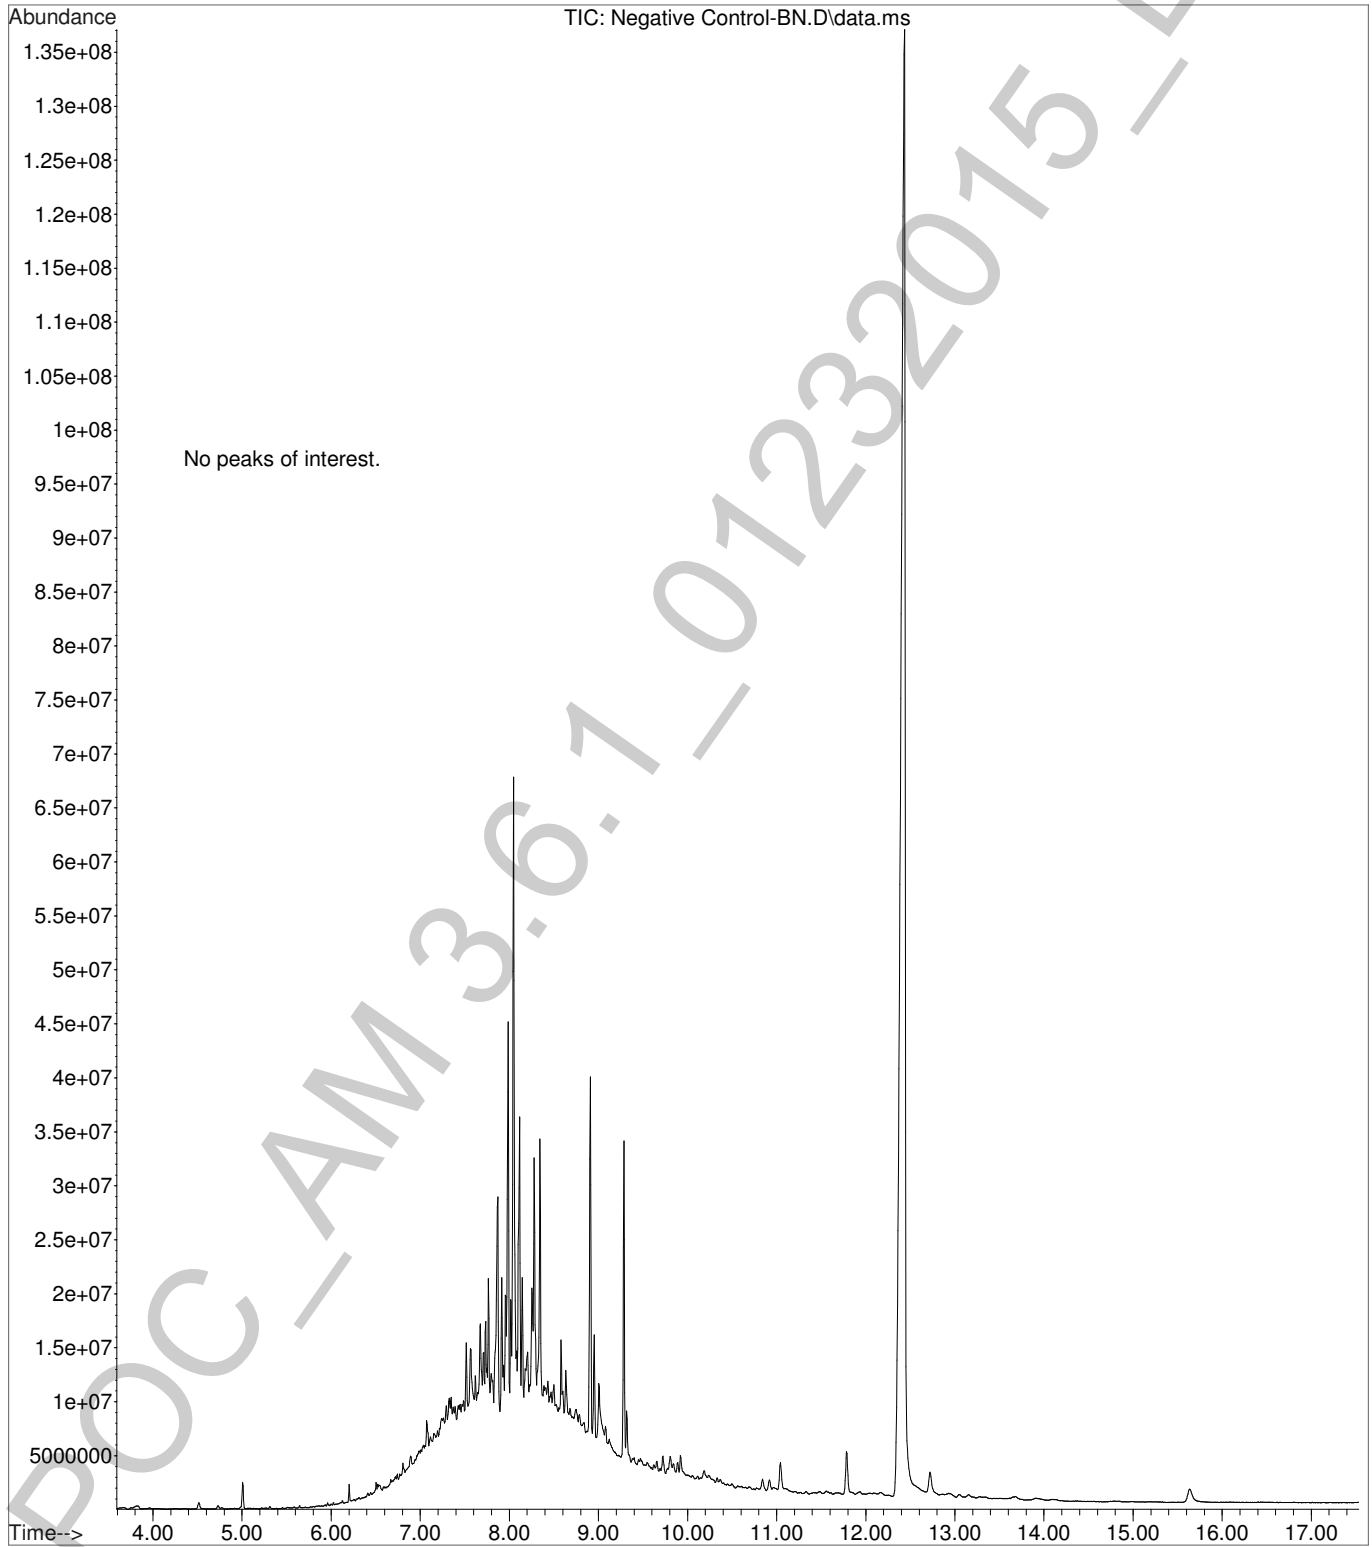


File :C:\gcms\1\data\Blood\012315BN\Negative Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 23 Jan 2015 17:12 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0130
Misc Info : Analytical Method 3.6.1
Vial Number: 1

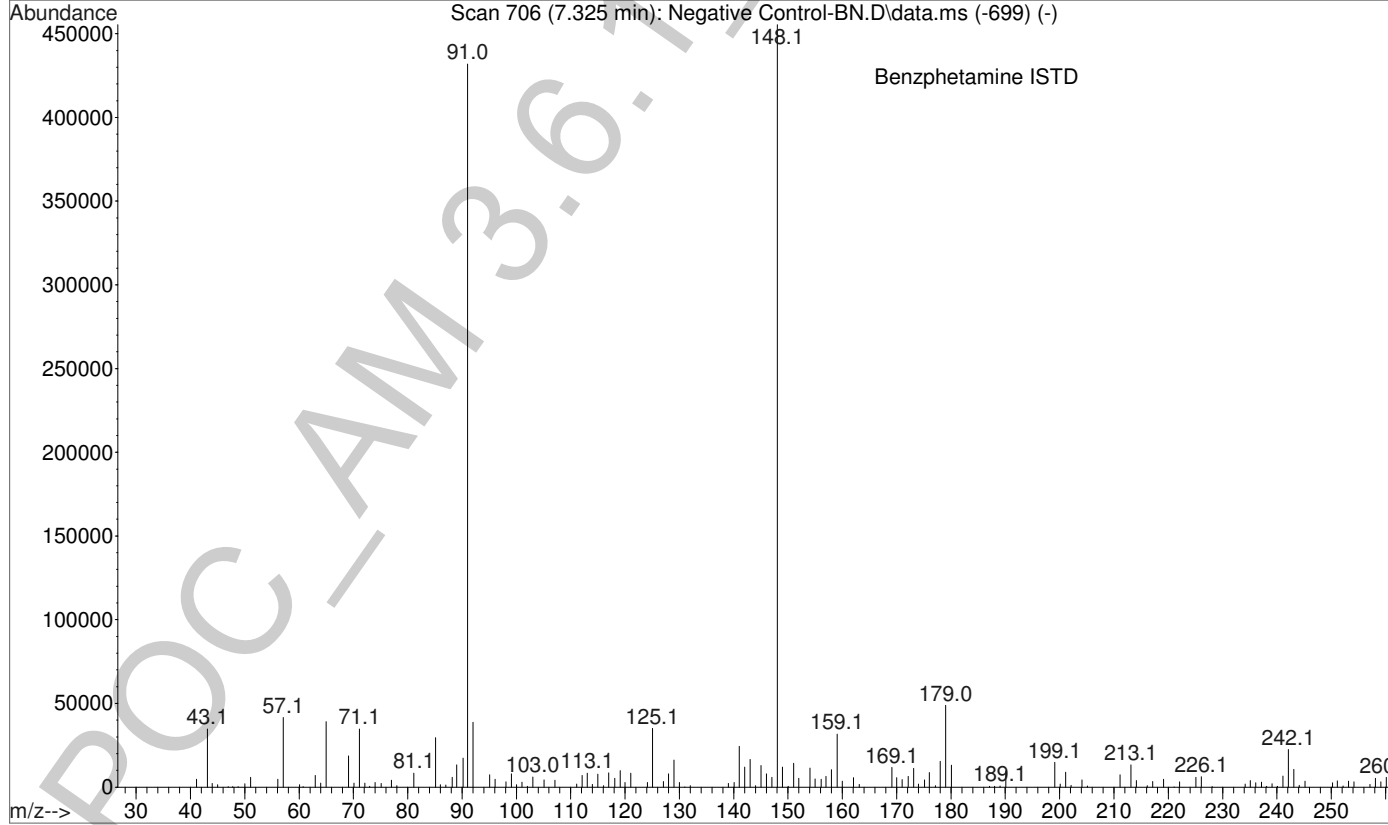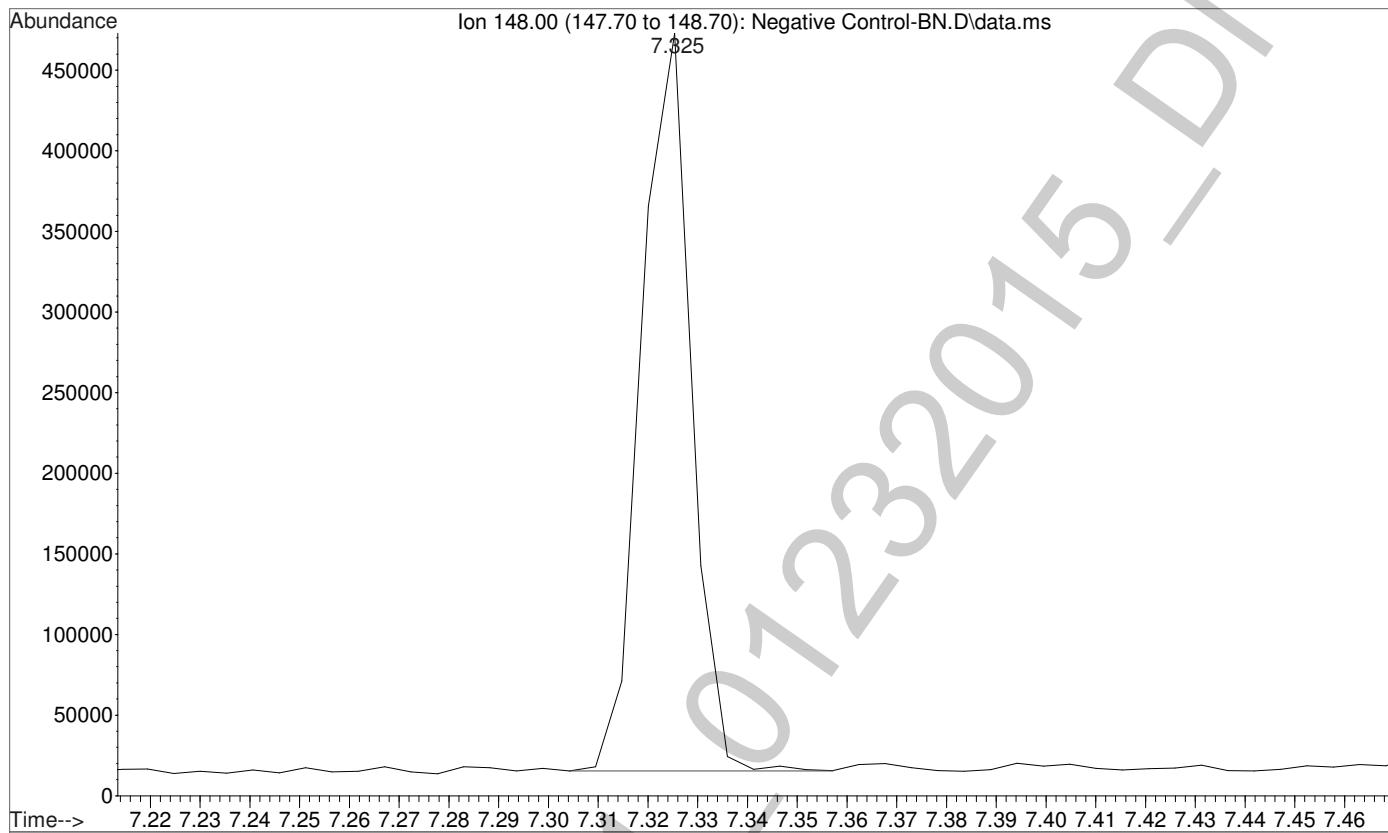



File :C:\gcms\1\data\Blood\012315BN\Negative Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 23 Jan 2015 17:12 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0130
Misc Info : Analytical Method 3.6.1
Vial Number: 1

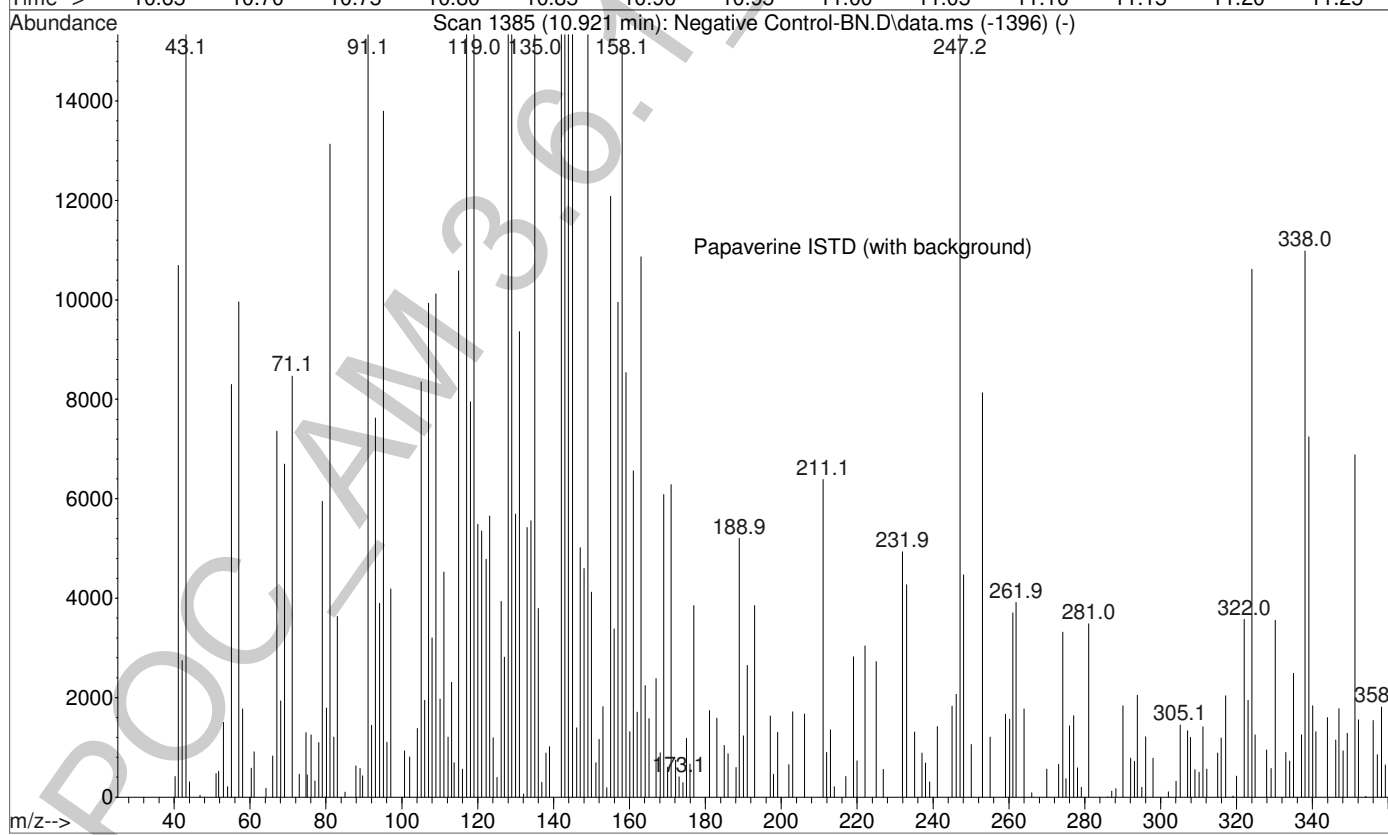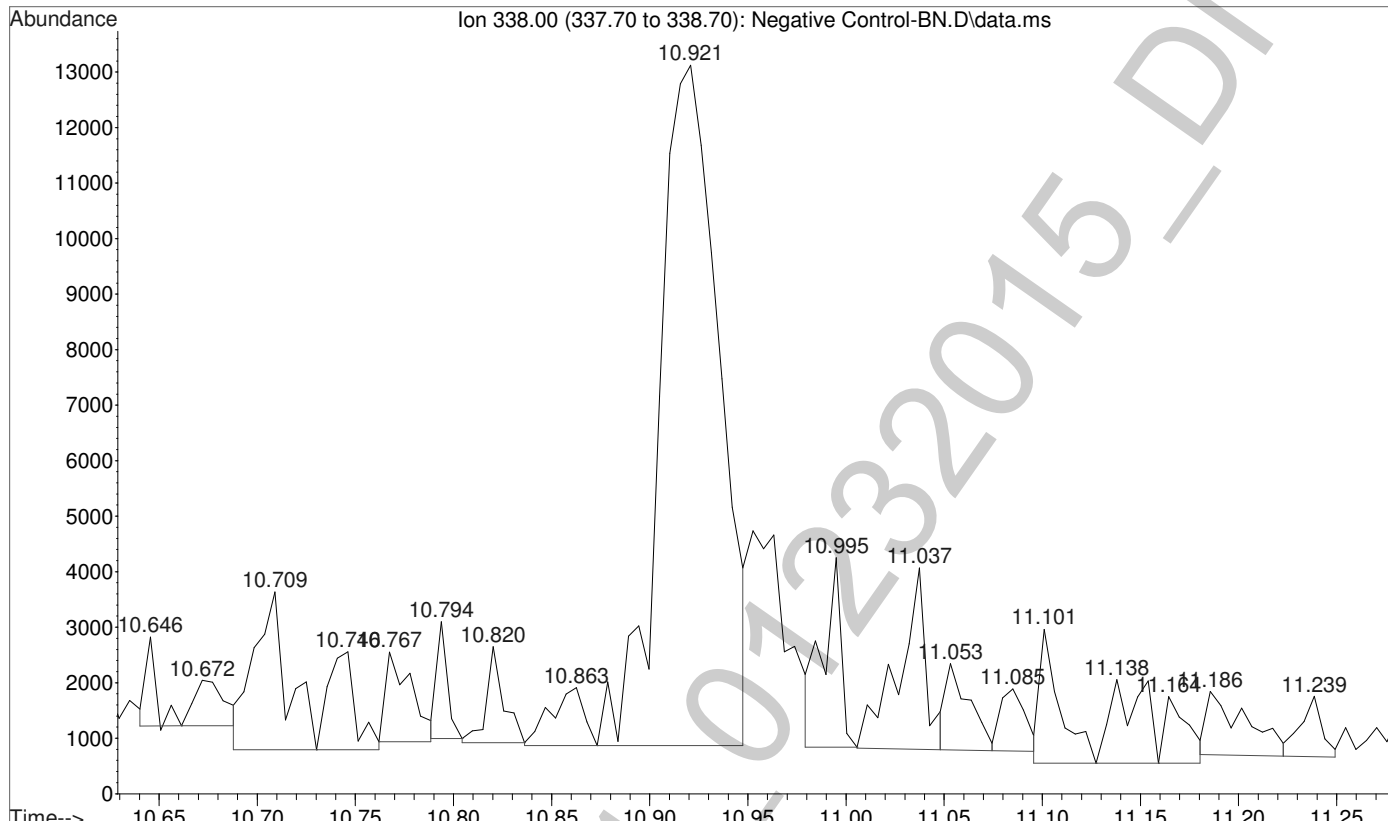



File :C:\gcms\1\data\Blood\012315BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 23 Jan 2015 17:35 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

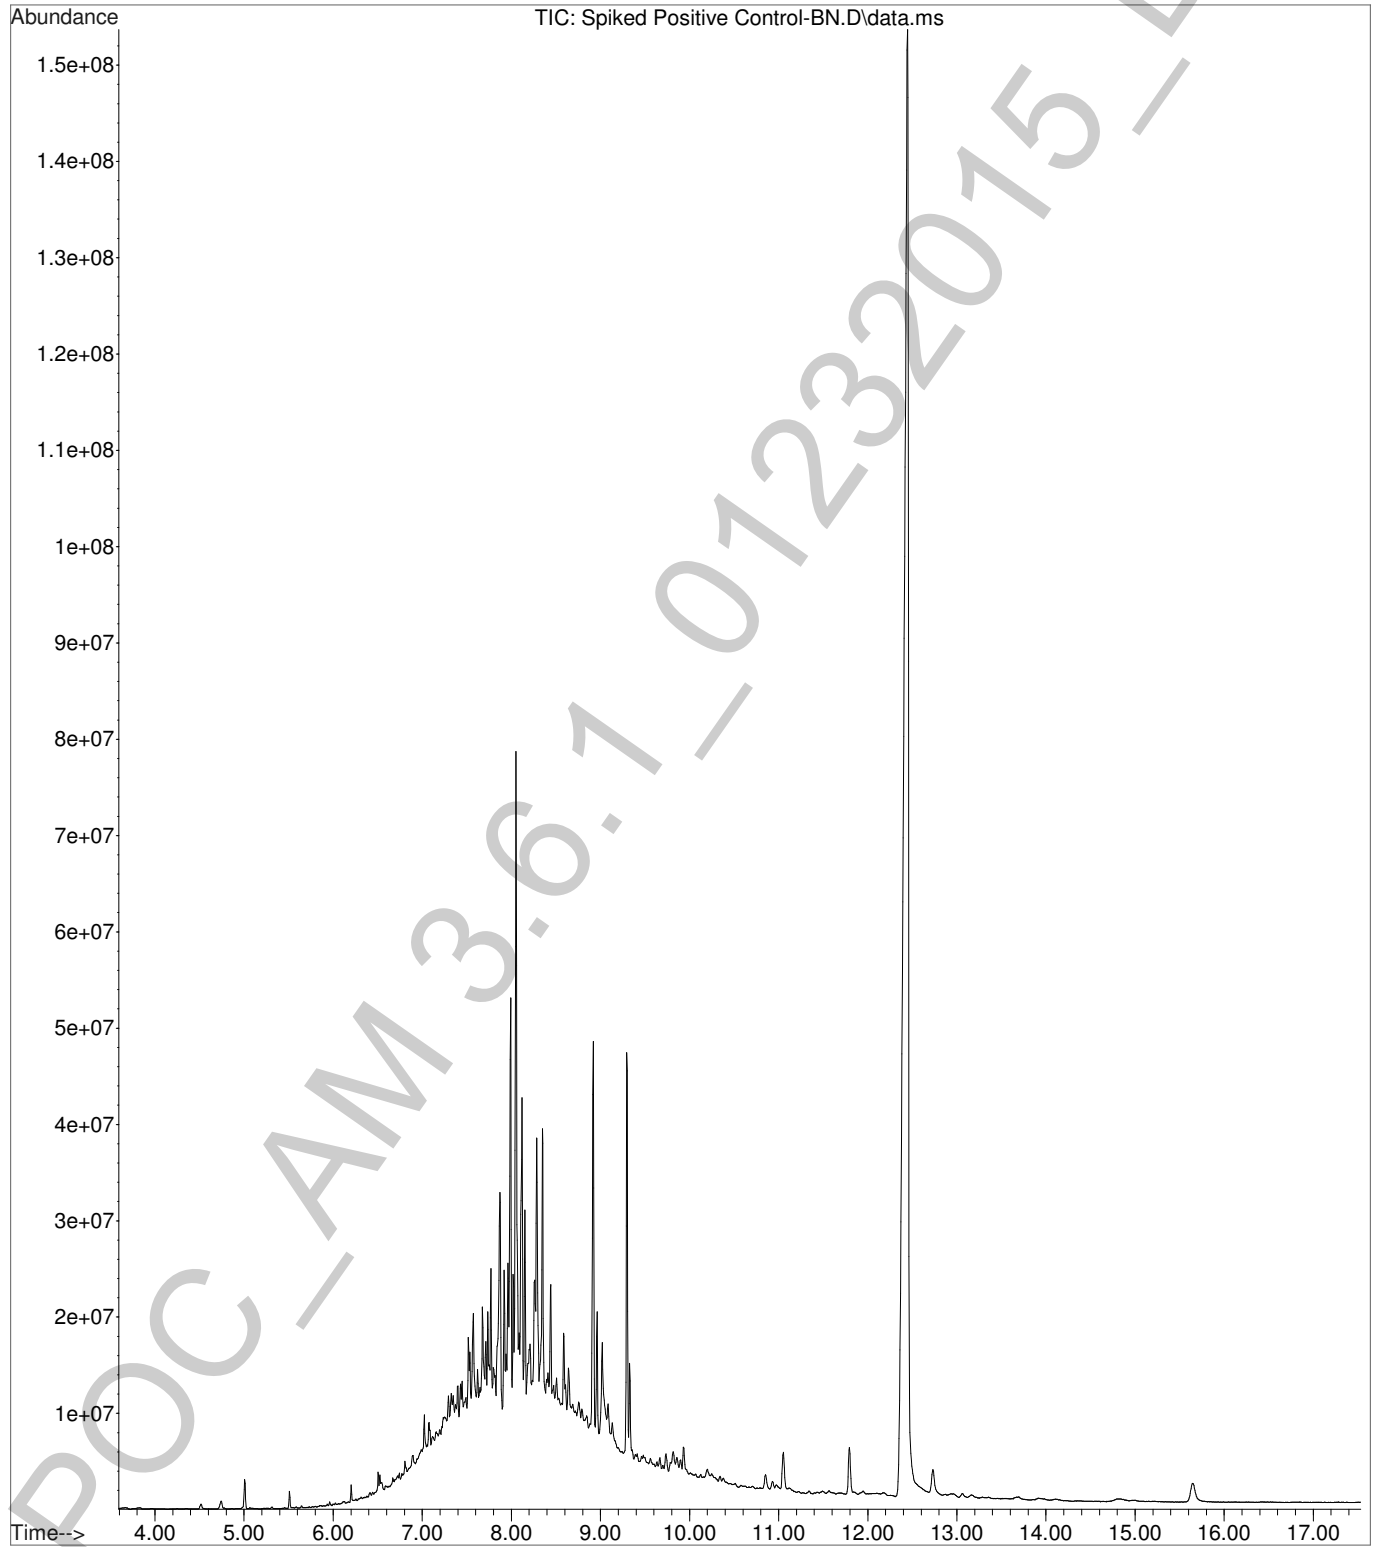



File :C:\gcms\1\data\Blood\012315BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 23 Jan 2015 17:35 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

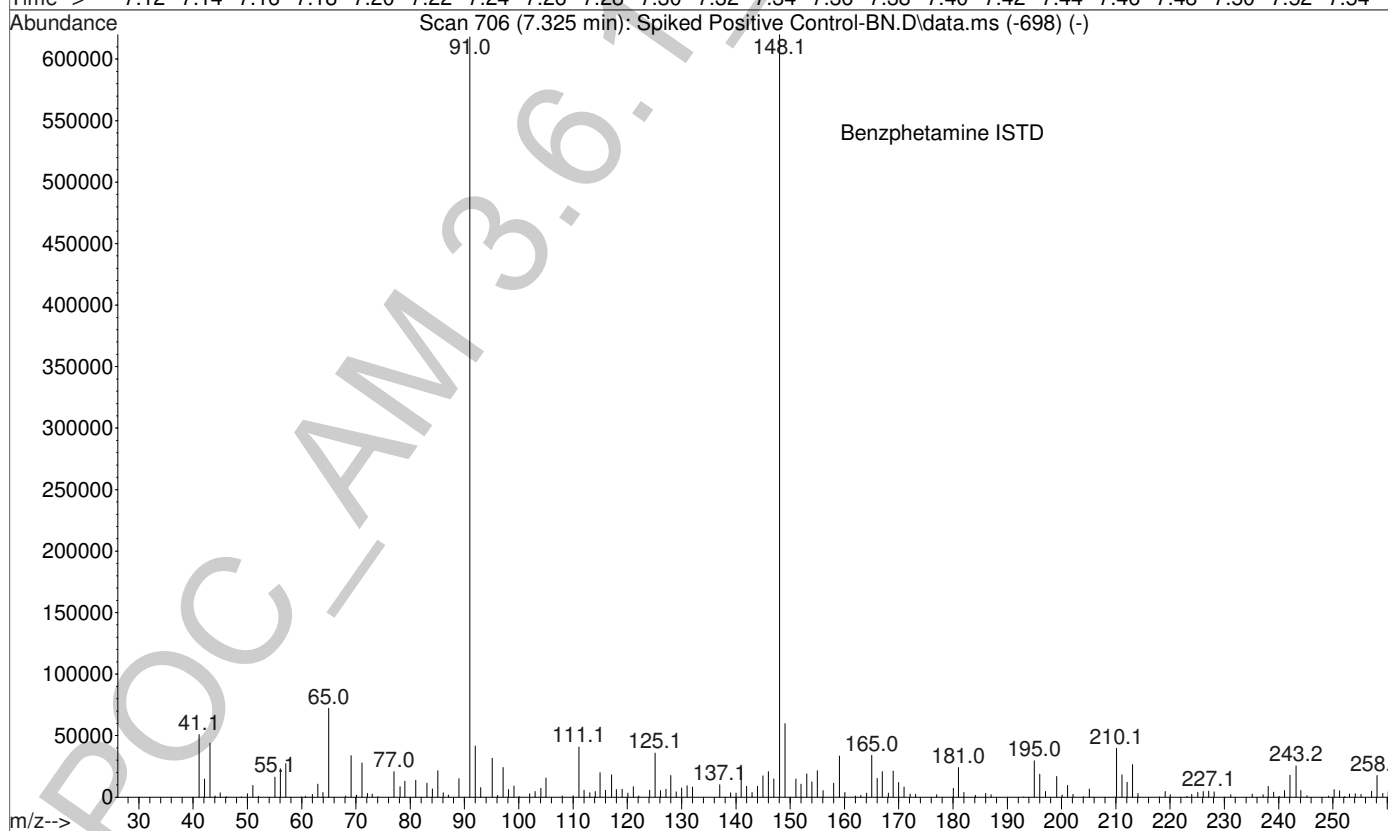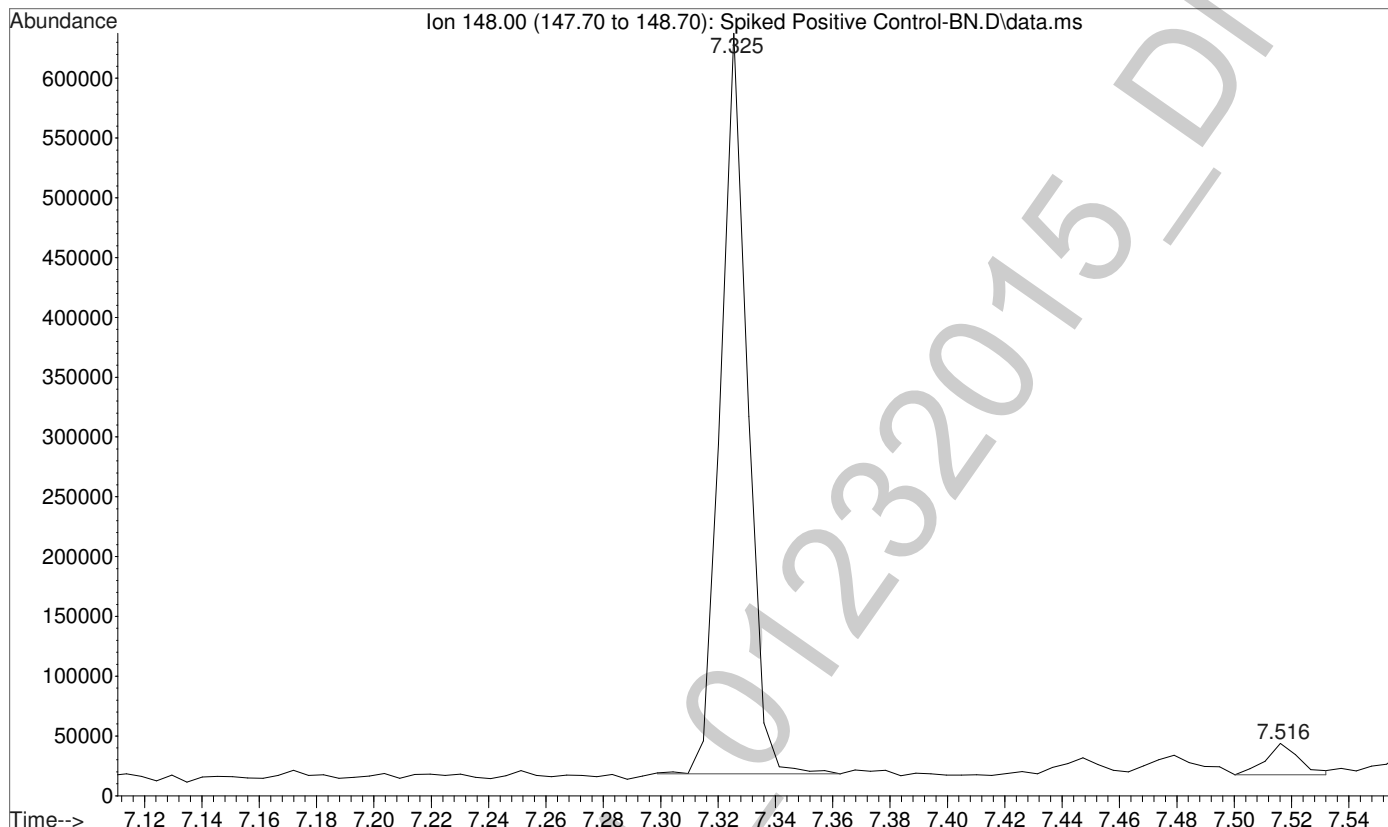



File :C:\gcms\1\data\Blood\012315BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 23 Jan 2015 17:35 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

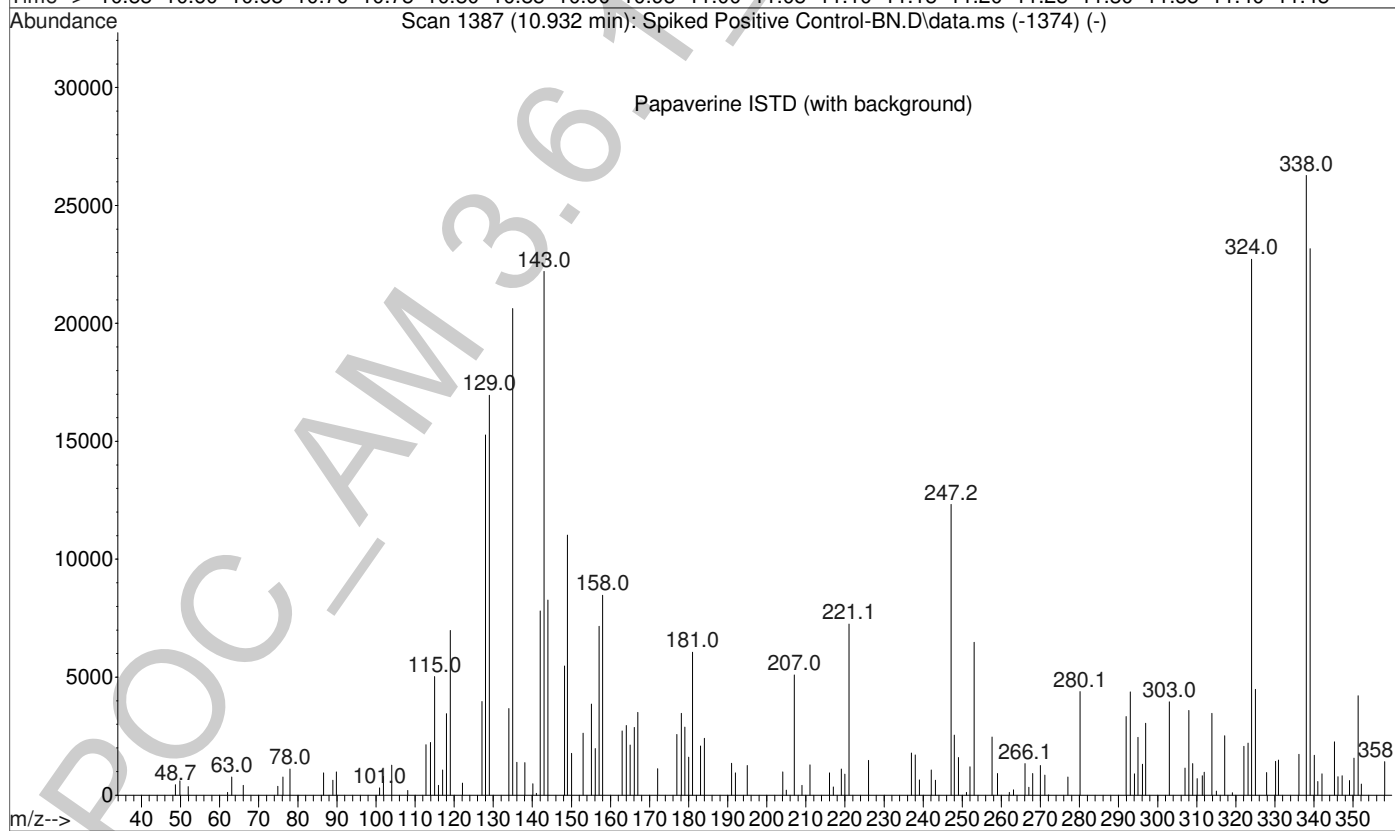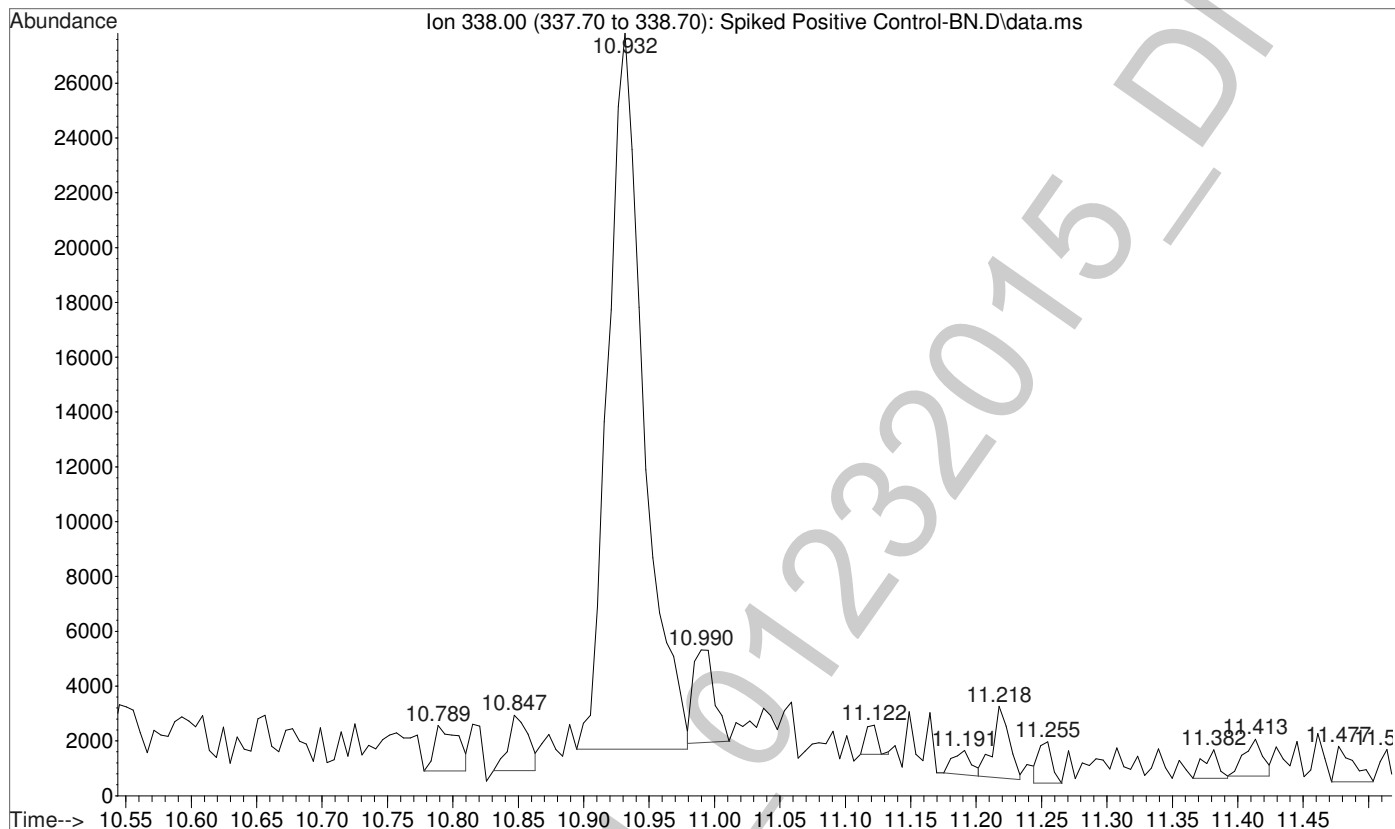



File :C:\gcms\1\data\Blood\012315BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 23 Jan 2015 17:35 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

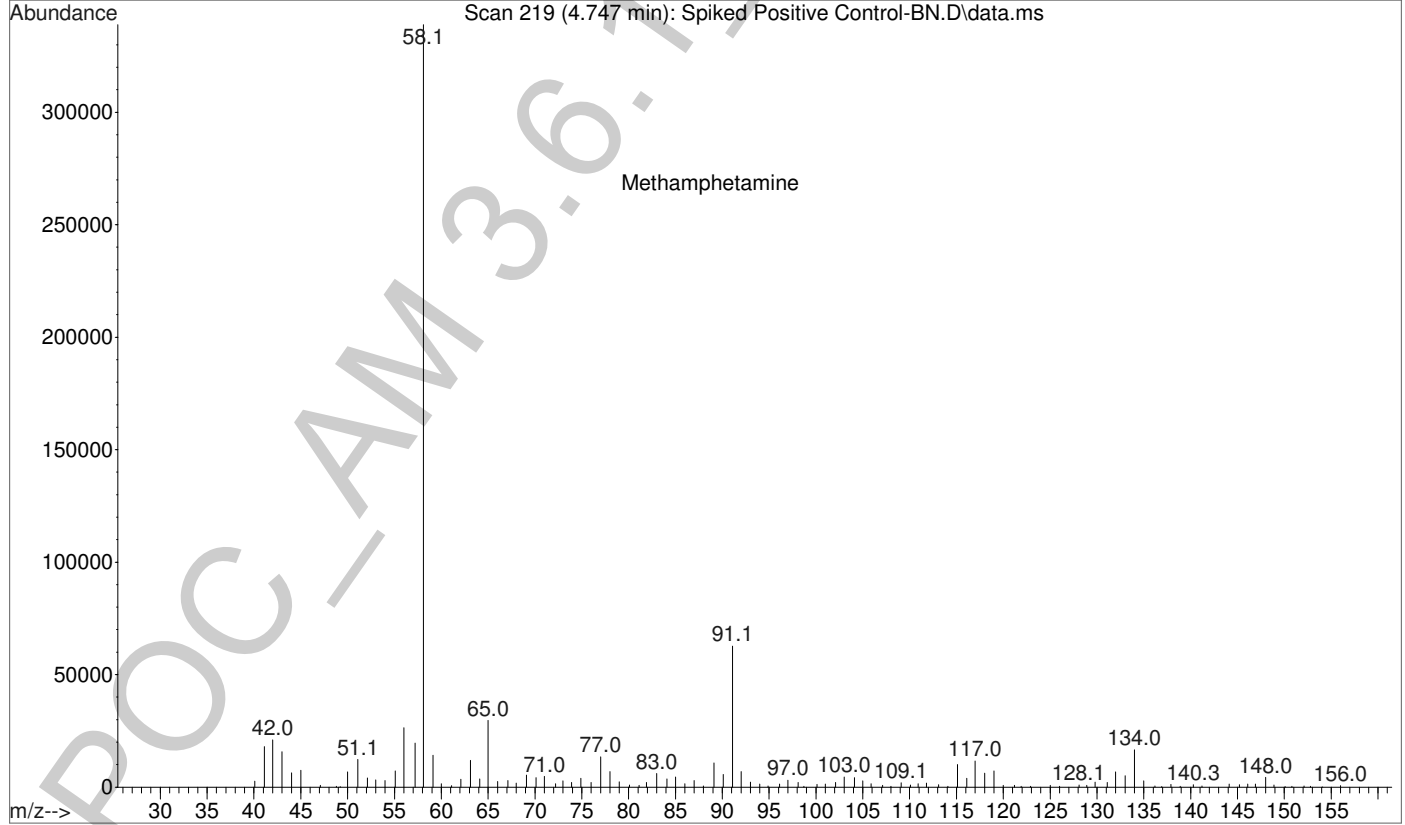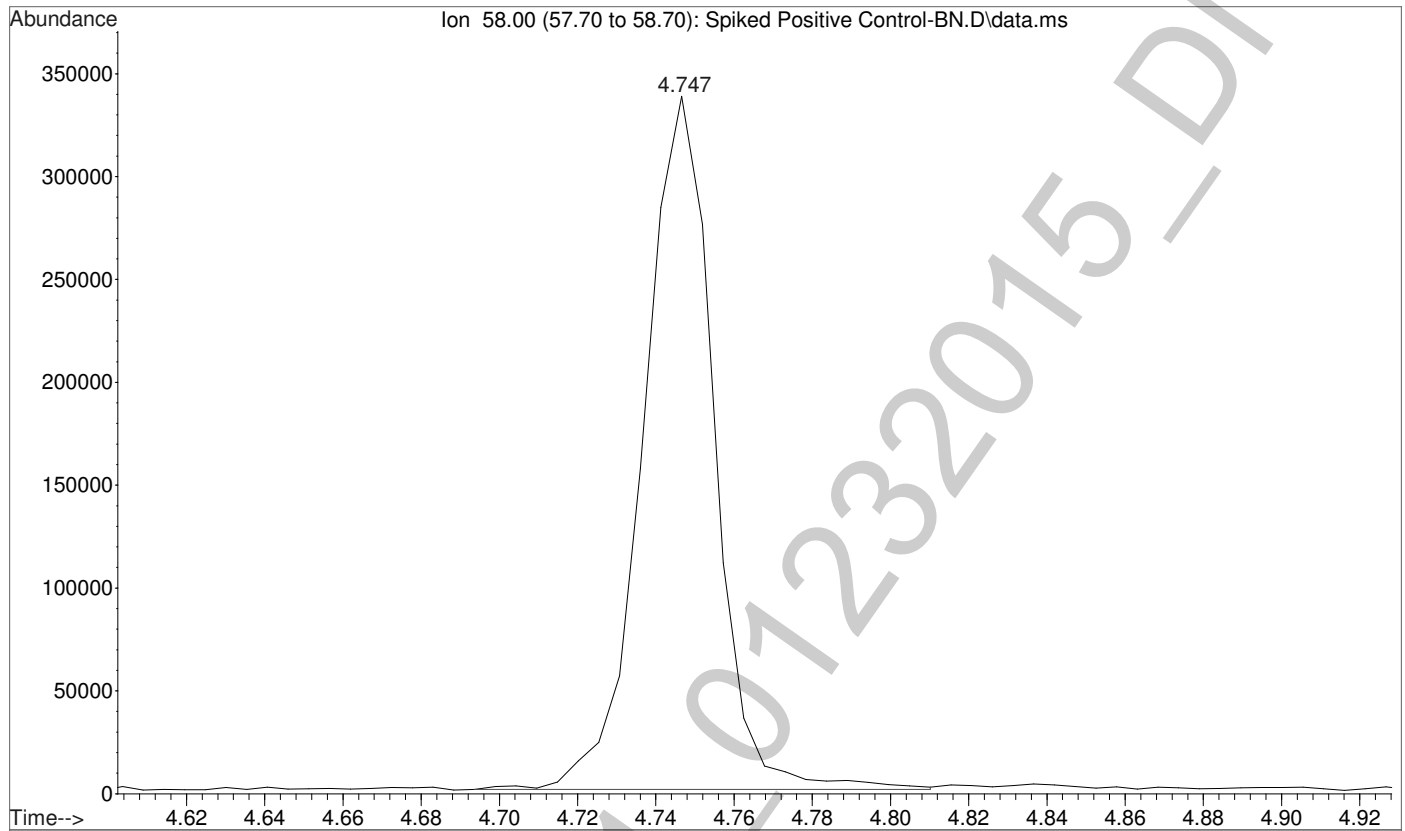



File :C:\gcms\1\data\Blood\012315BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 23 Jan 2015 17:35 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

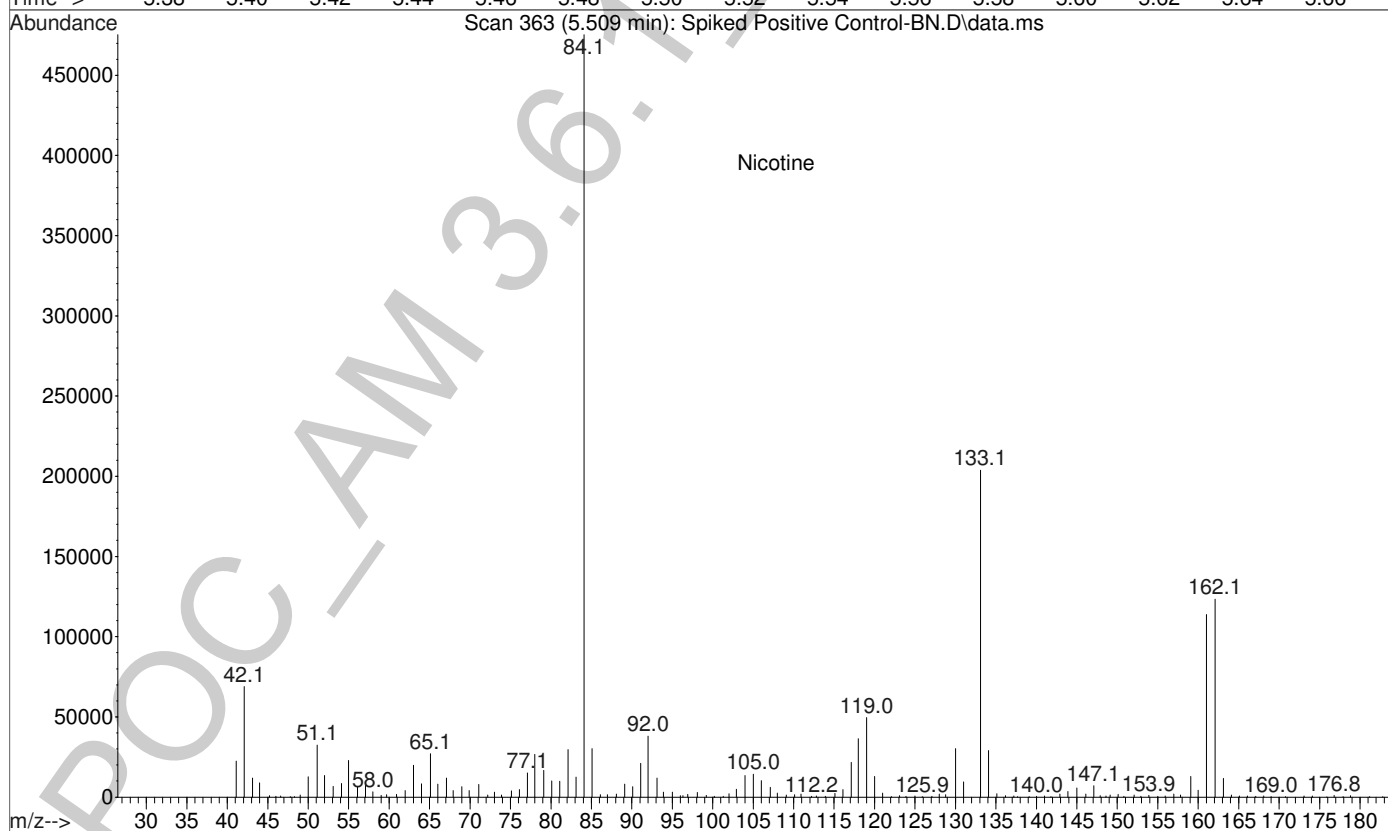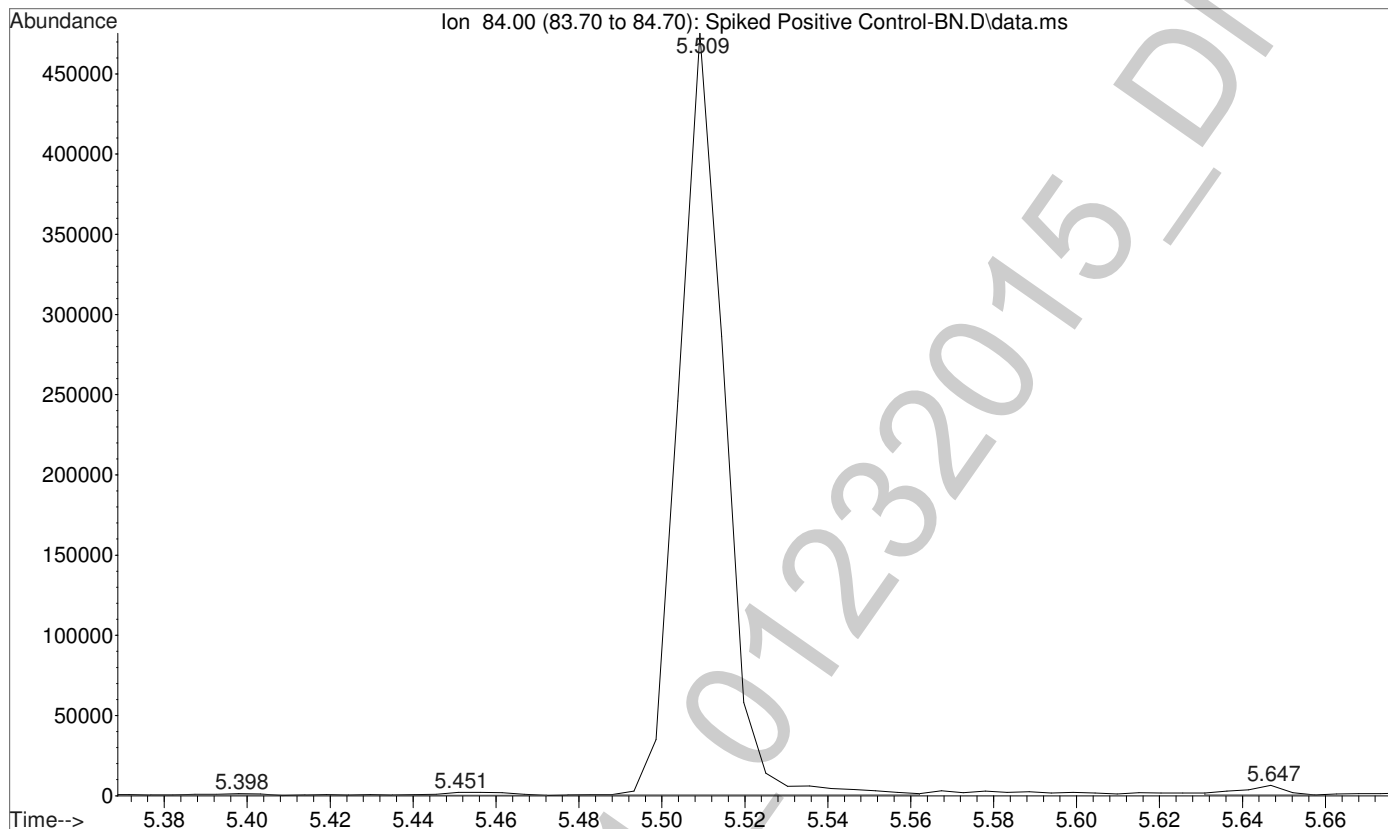



File :C:\gcms\1\data\Blood\012315BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 23 Jan 2015 17:35 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

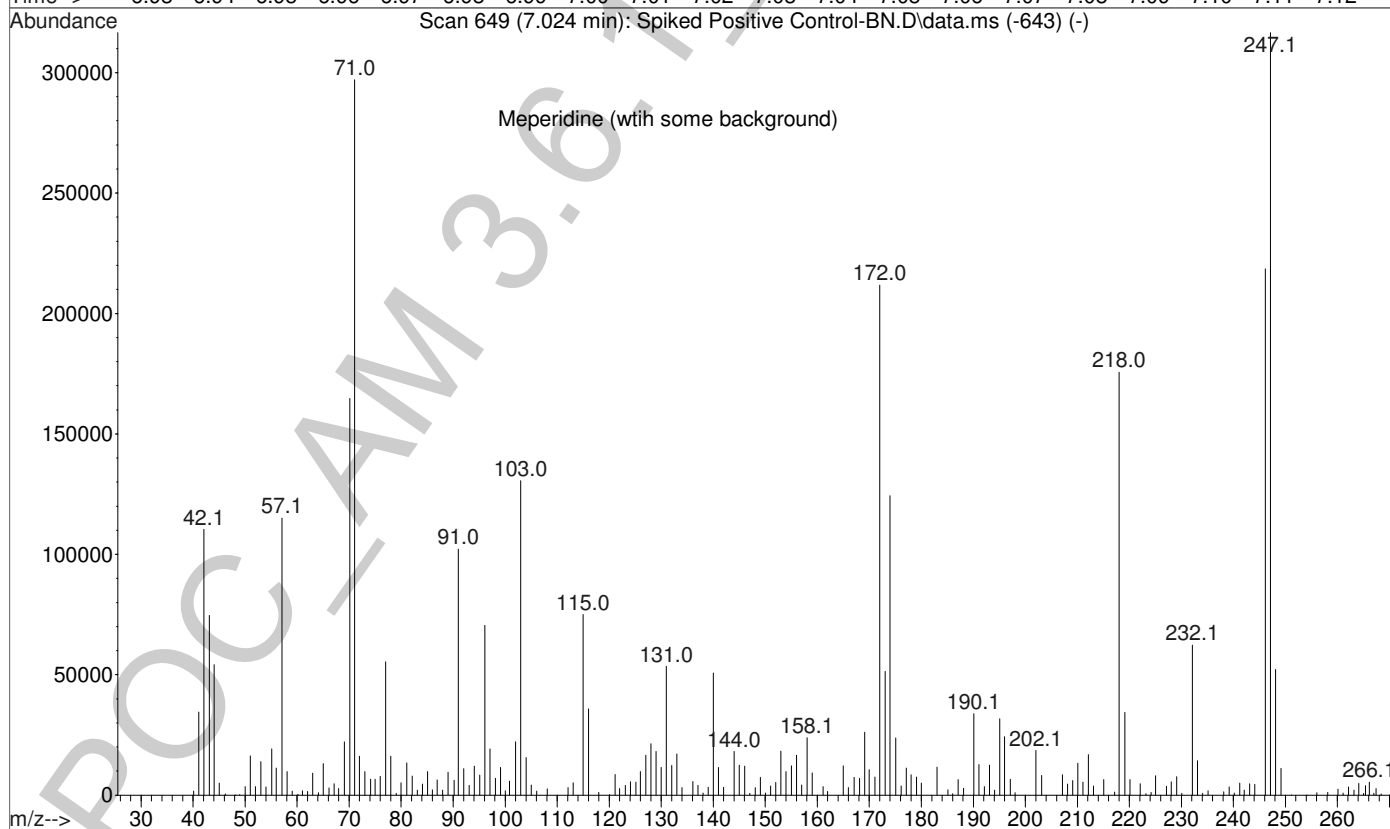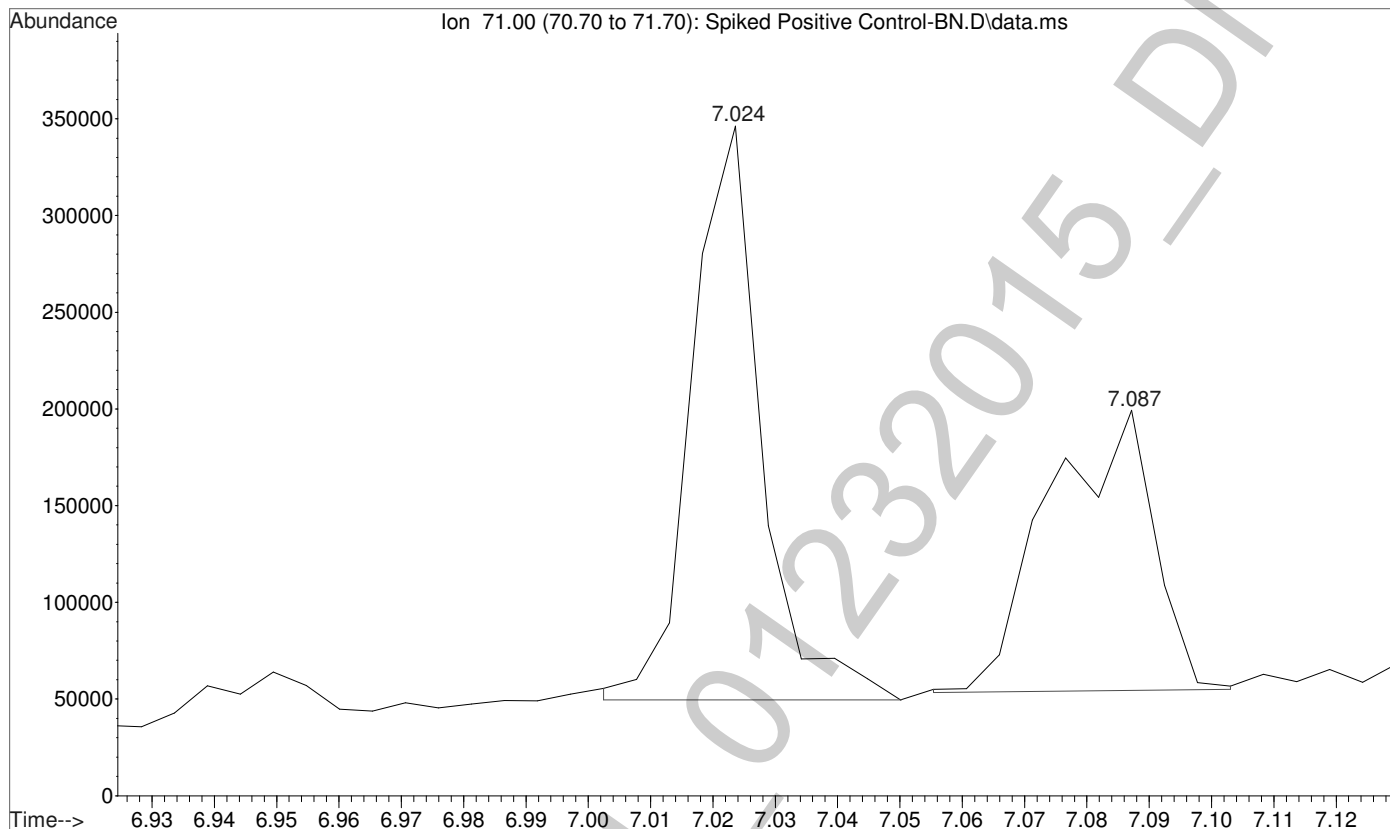



File :C:\gcms\1\data\Blood\012315BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 23 Jan 2015 17:35 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

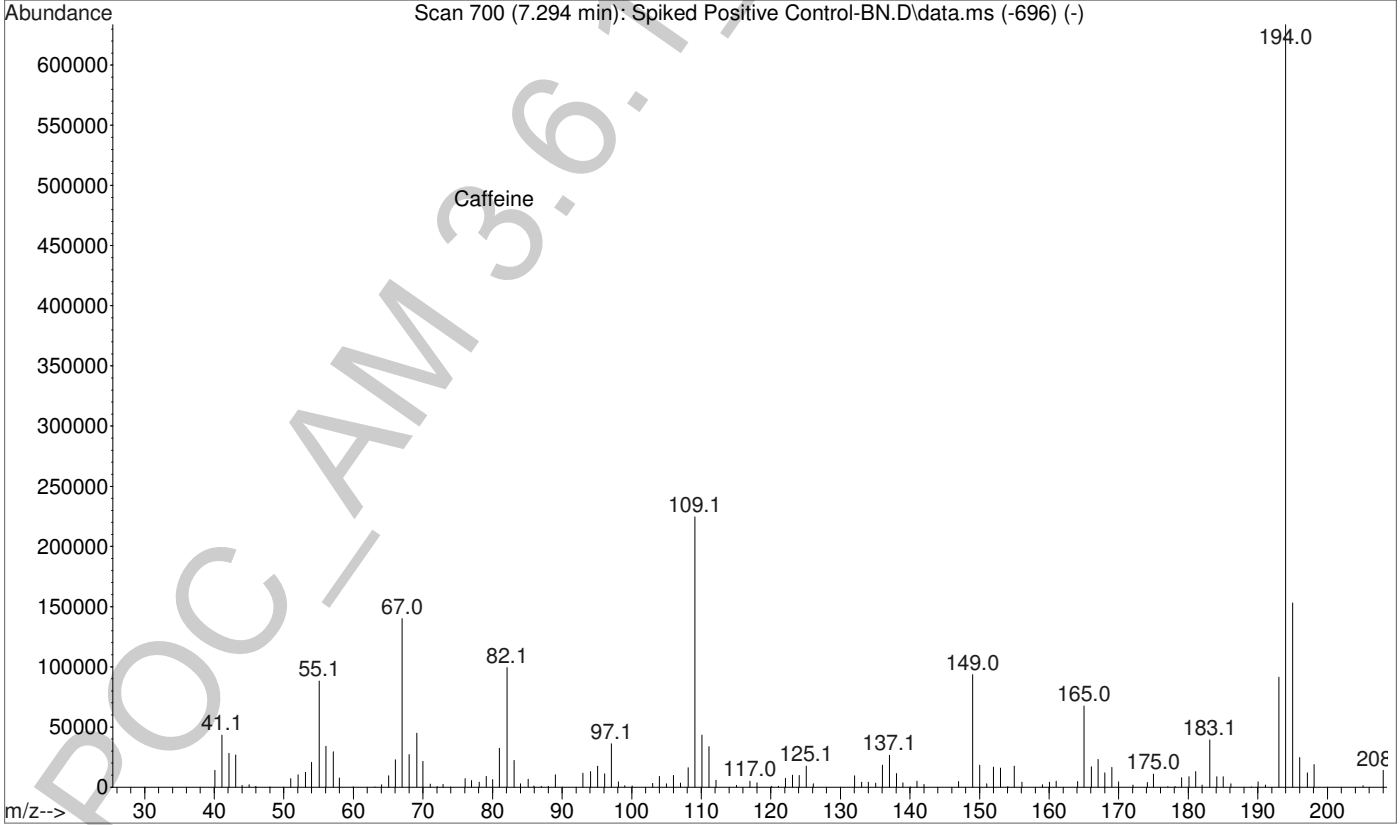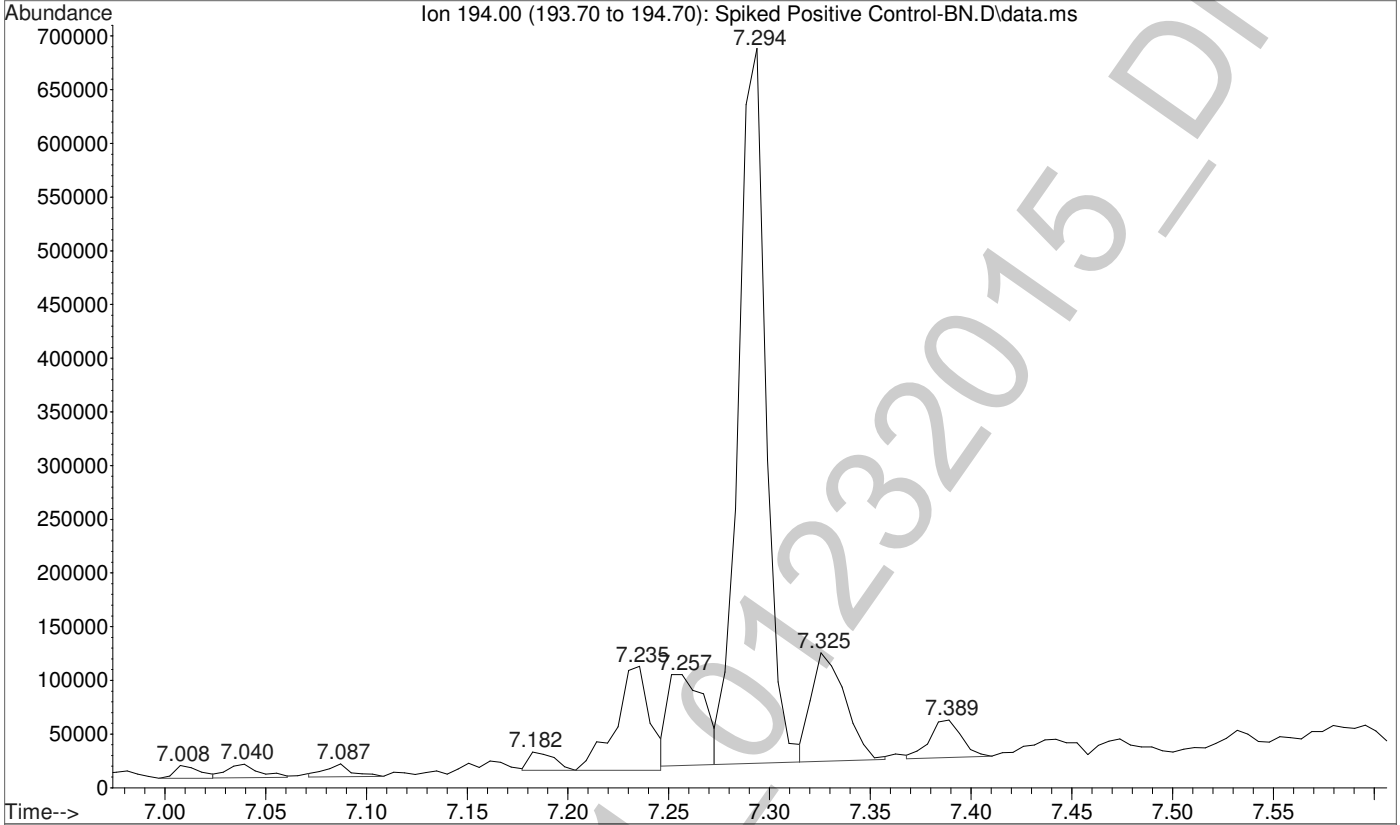




File :C:\gcms\1\data\Blood\012315BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 23 Jan 2015 17:35 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

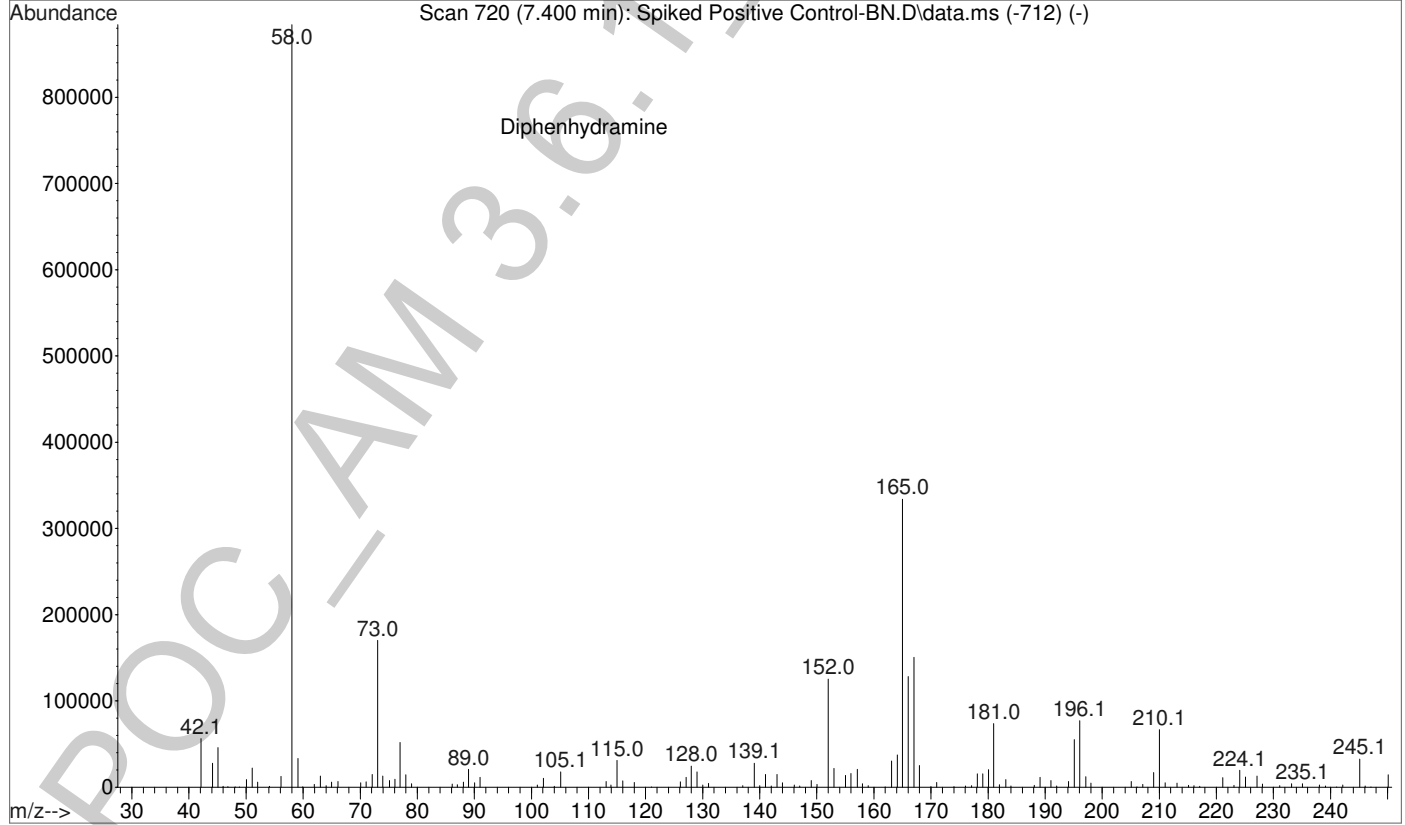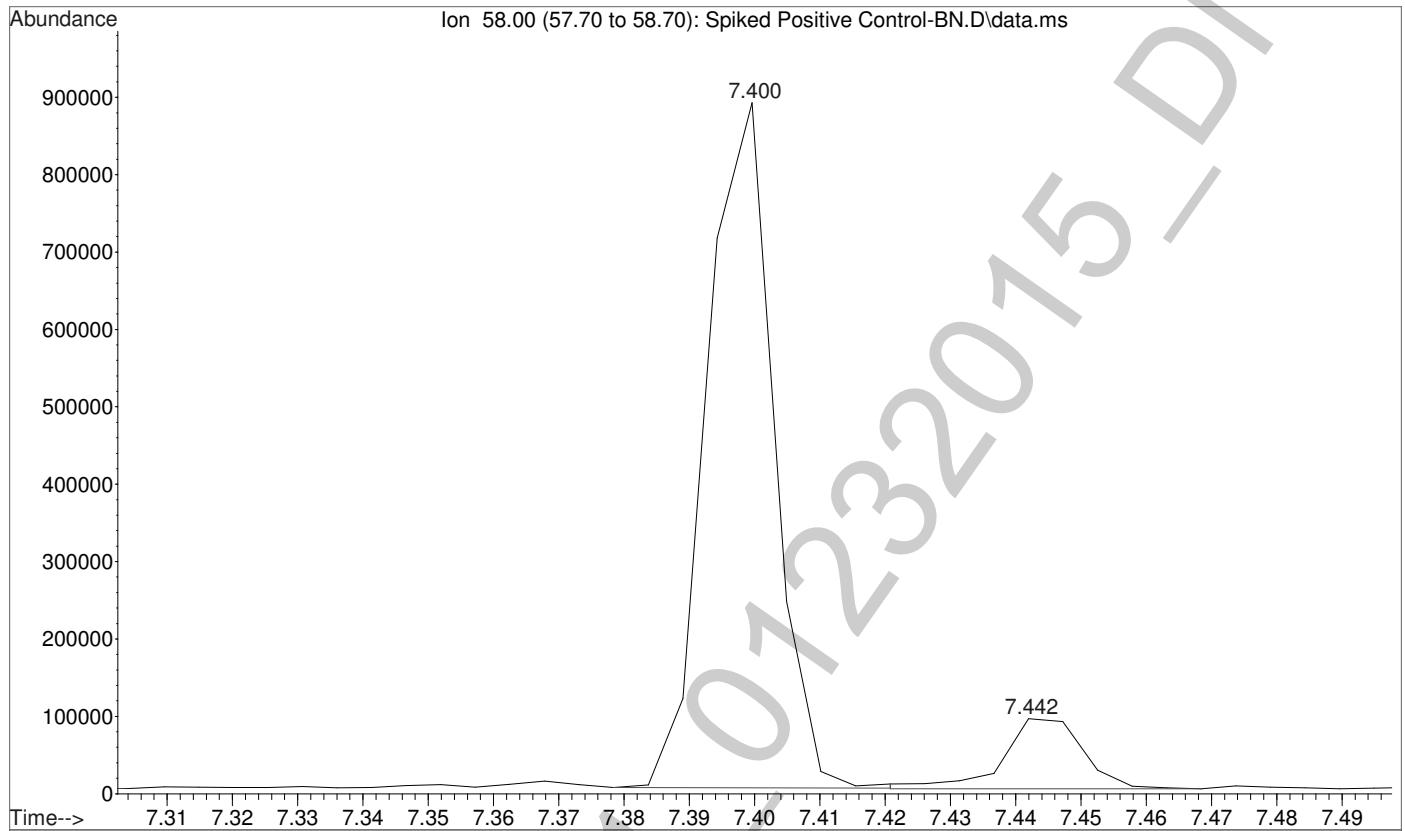



File :C:\gcms\1\data\Blood\012315BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 23 Jan 2015 17:35 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

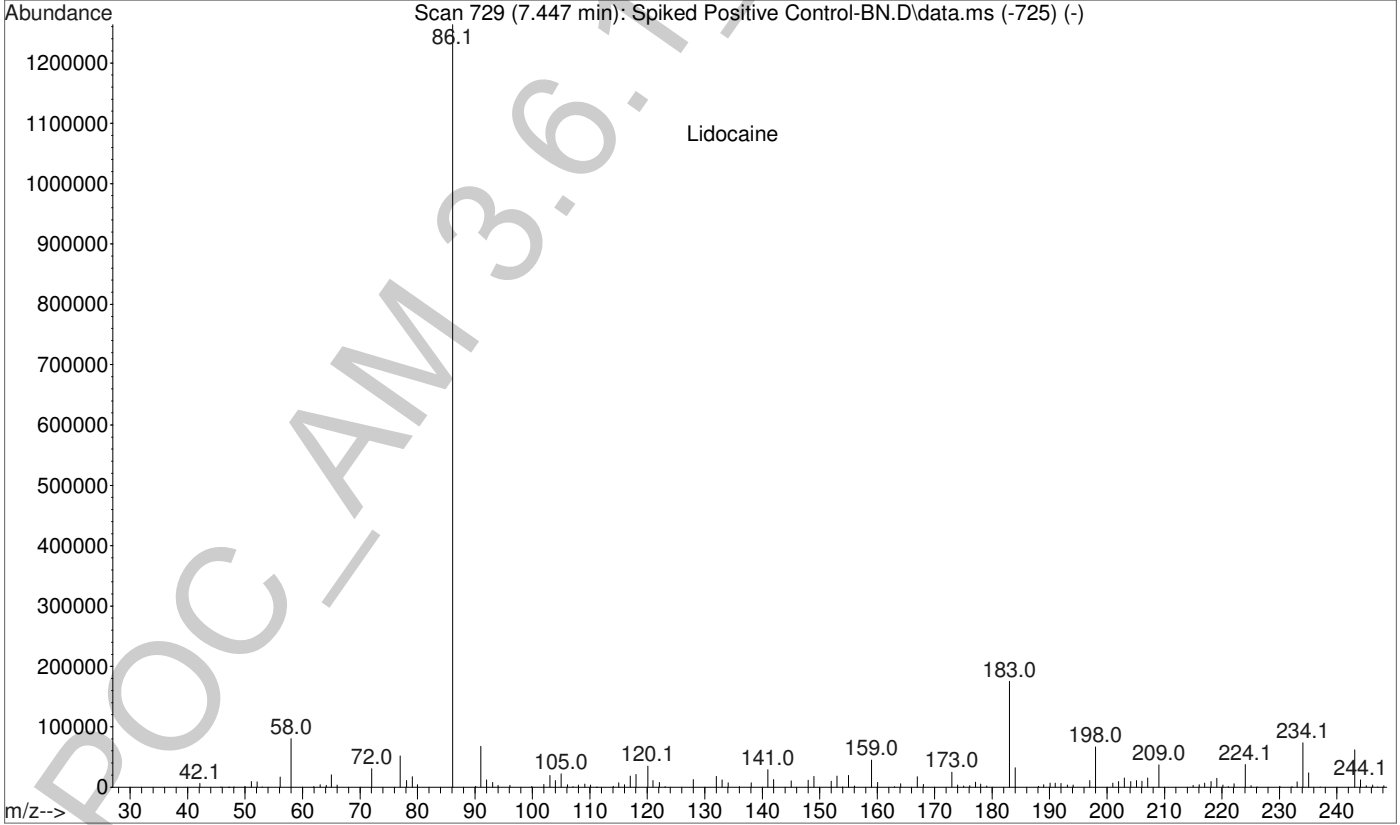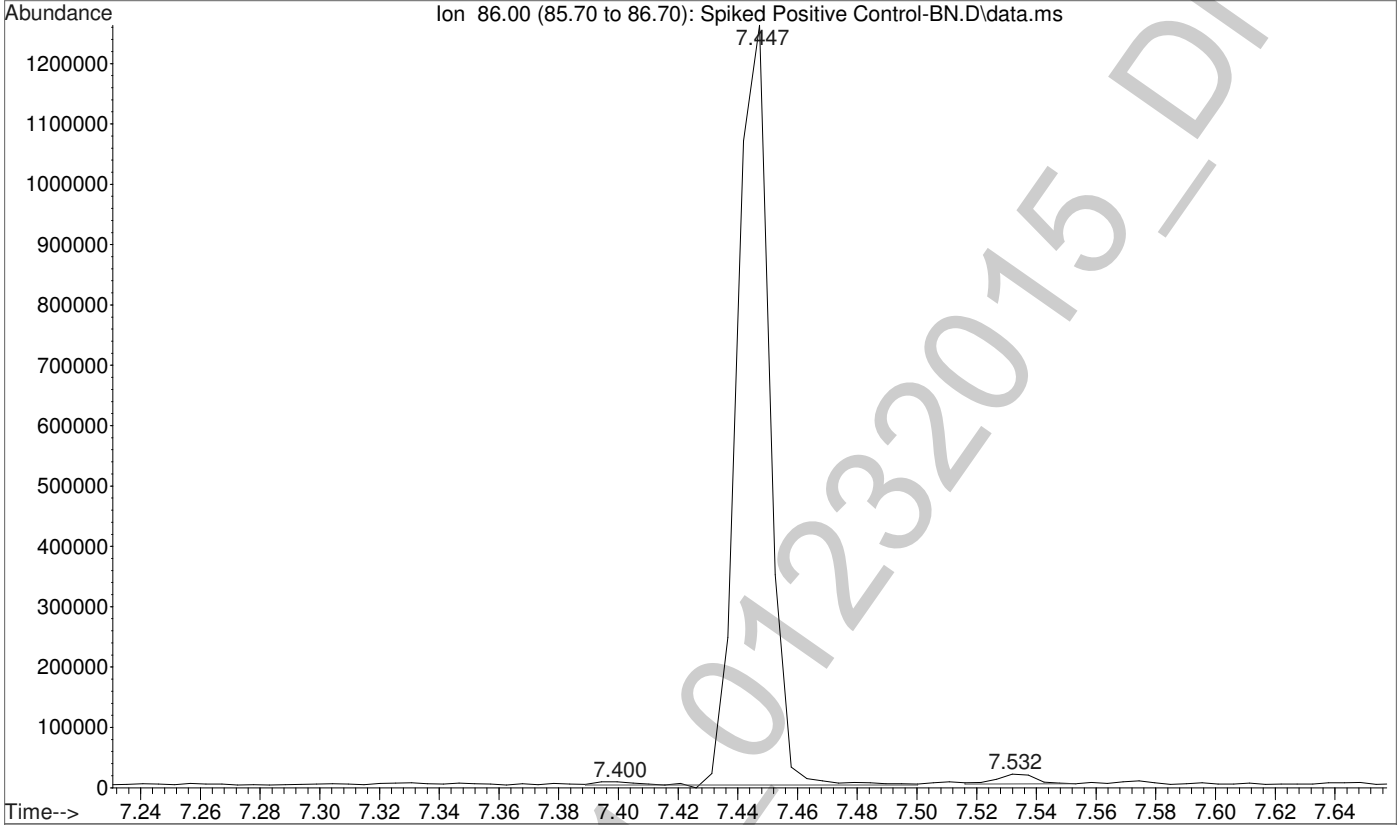




File :C:\gcms\1\data\Blood\012315BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 23 Jan 2015 17:35 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

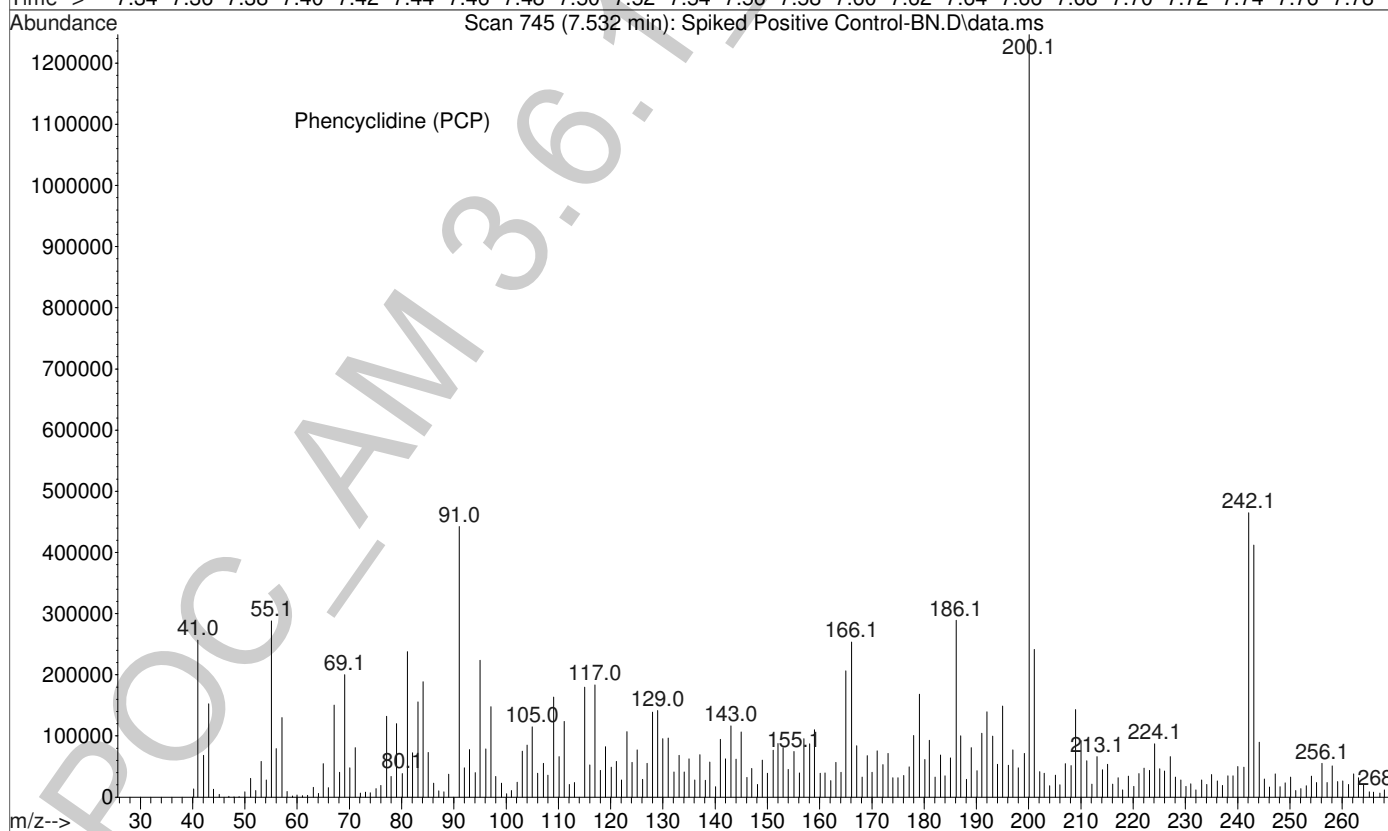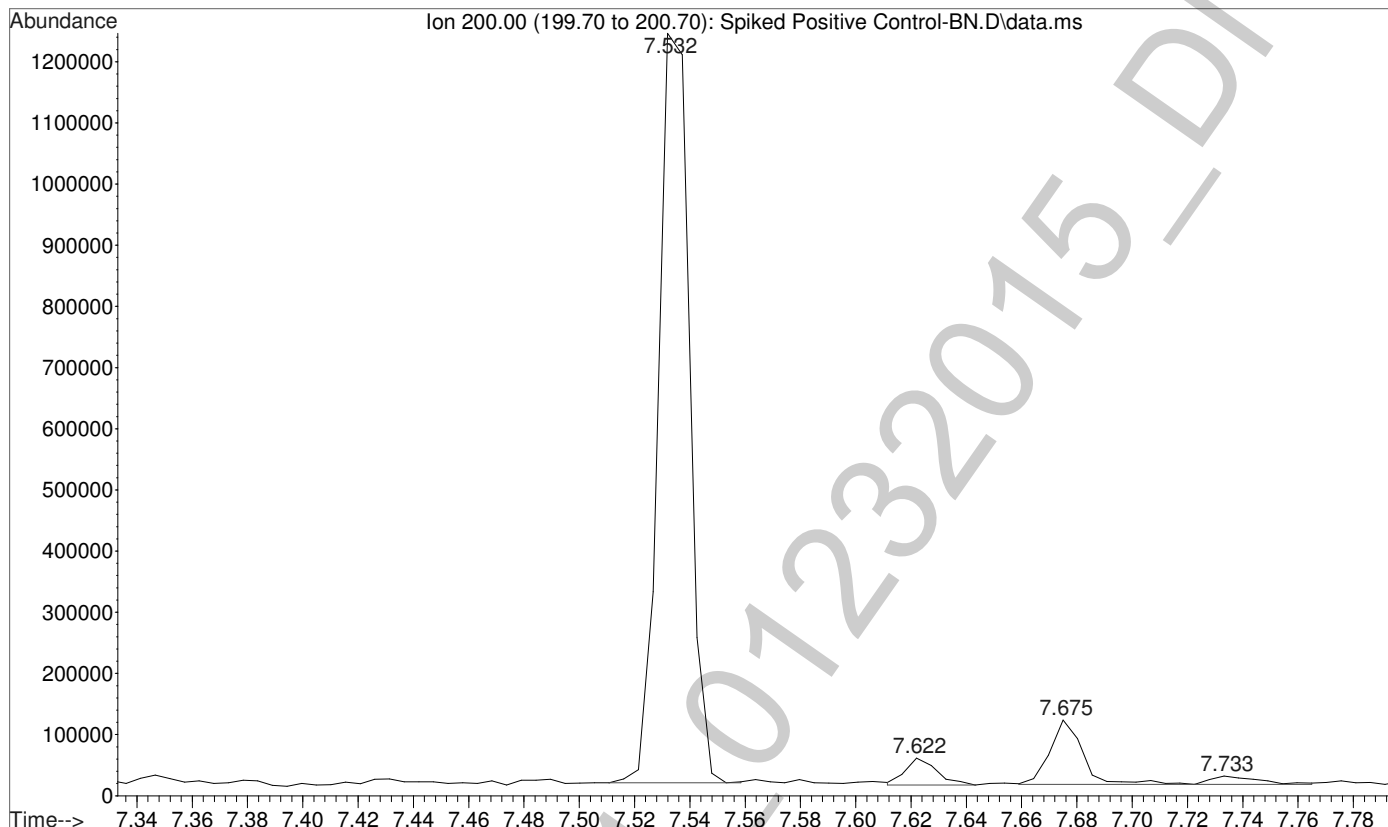



File :C:\gcms\1\data\Blood\012315BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 23 Jan 2015 17:35 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

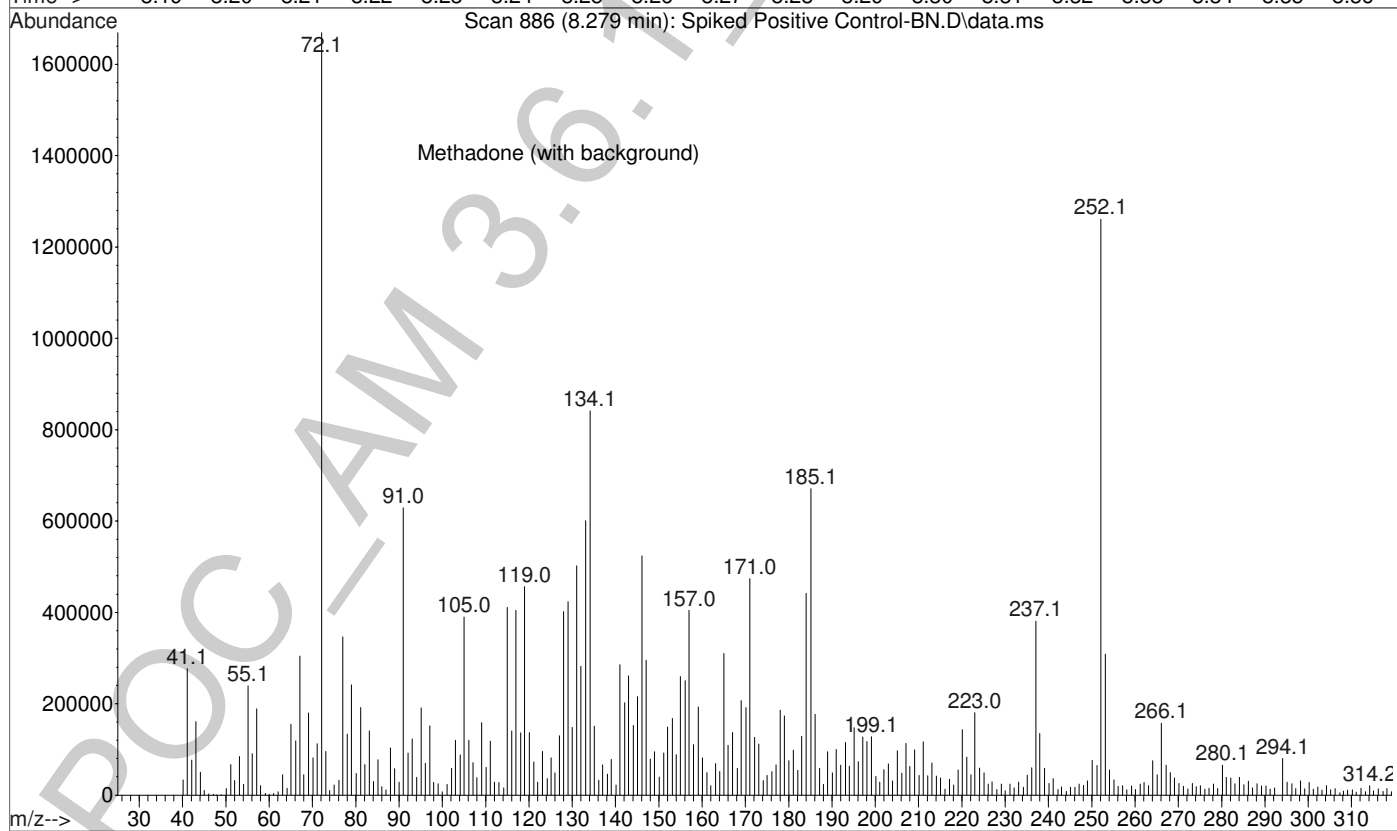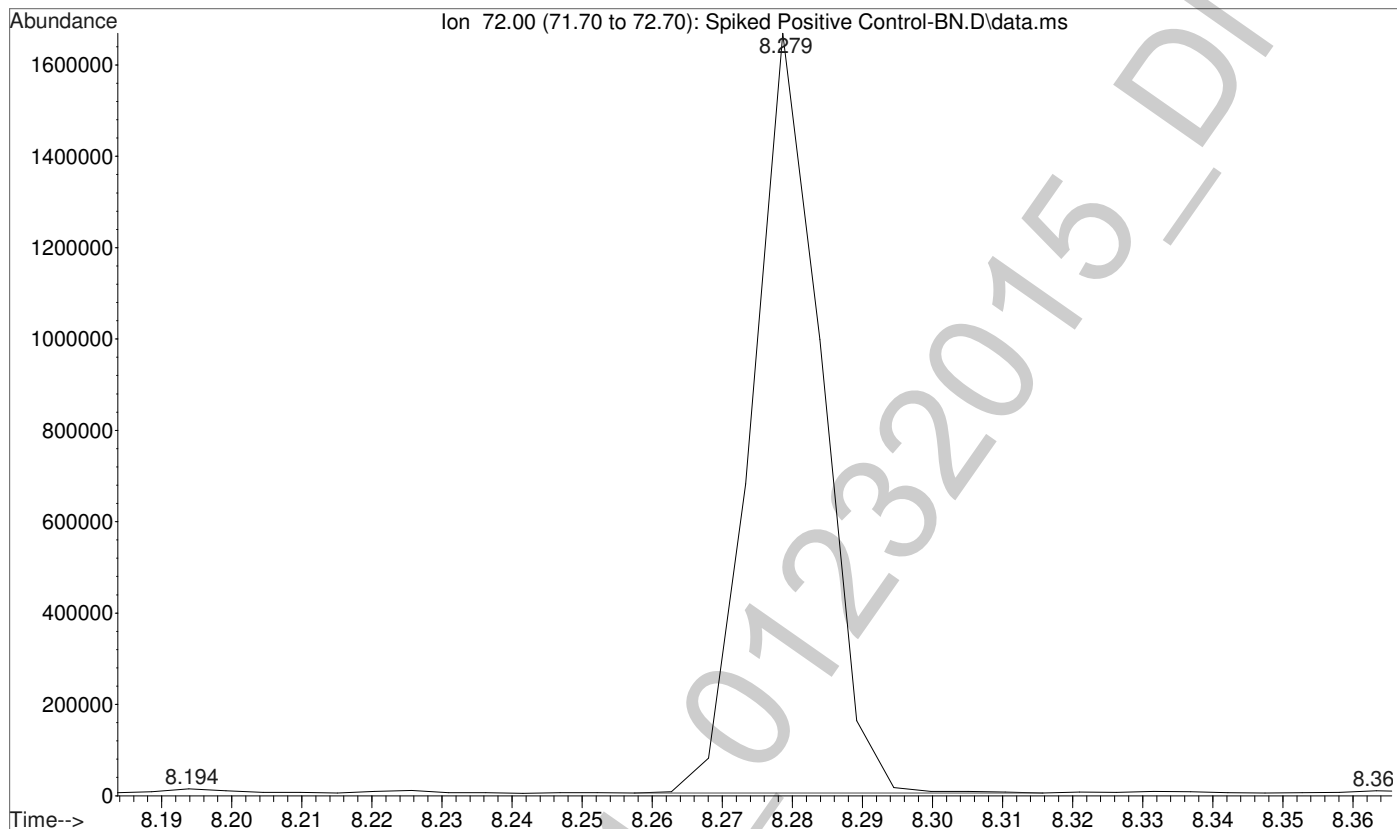



File :C:\gcms\1\data\Blood\012315BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 23 Jan 2015 17:35 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

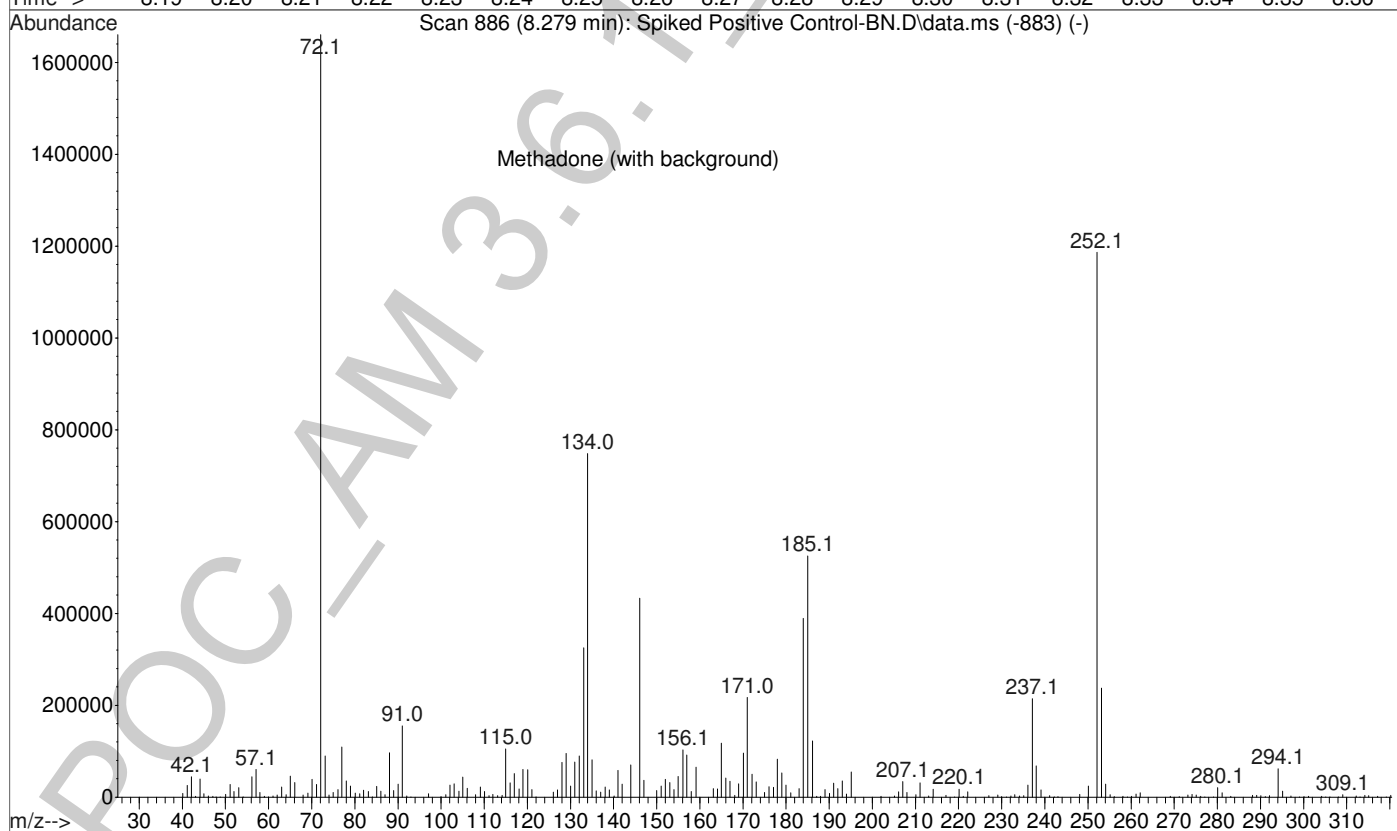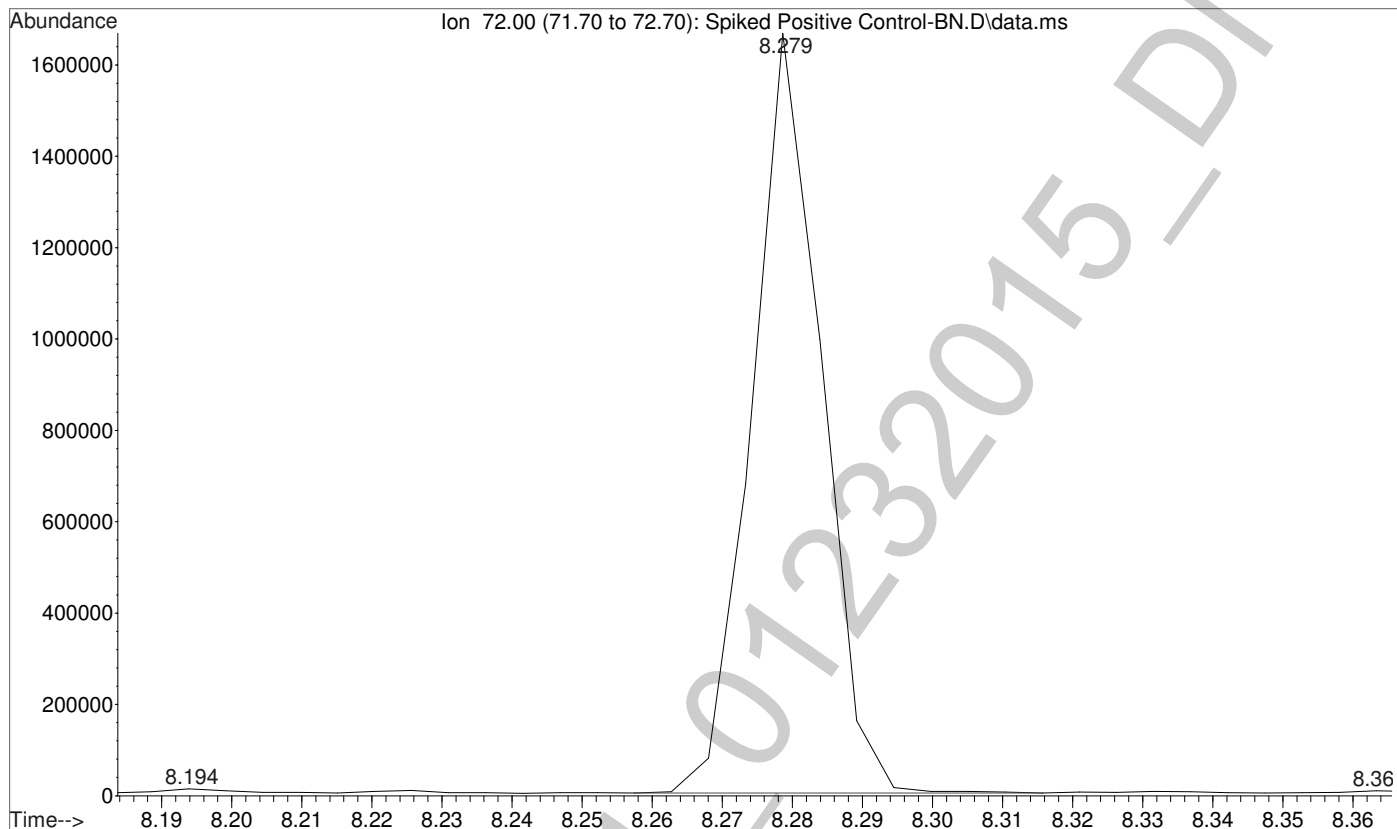



File :C:\gcms\1\data\Blood\012315BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 23 Jan 2015 17:35 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

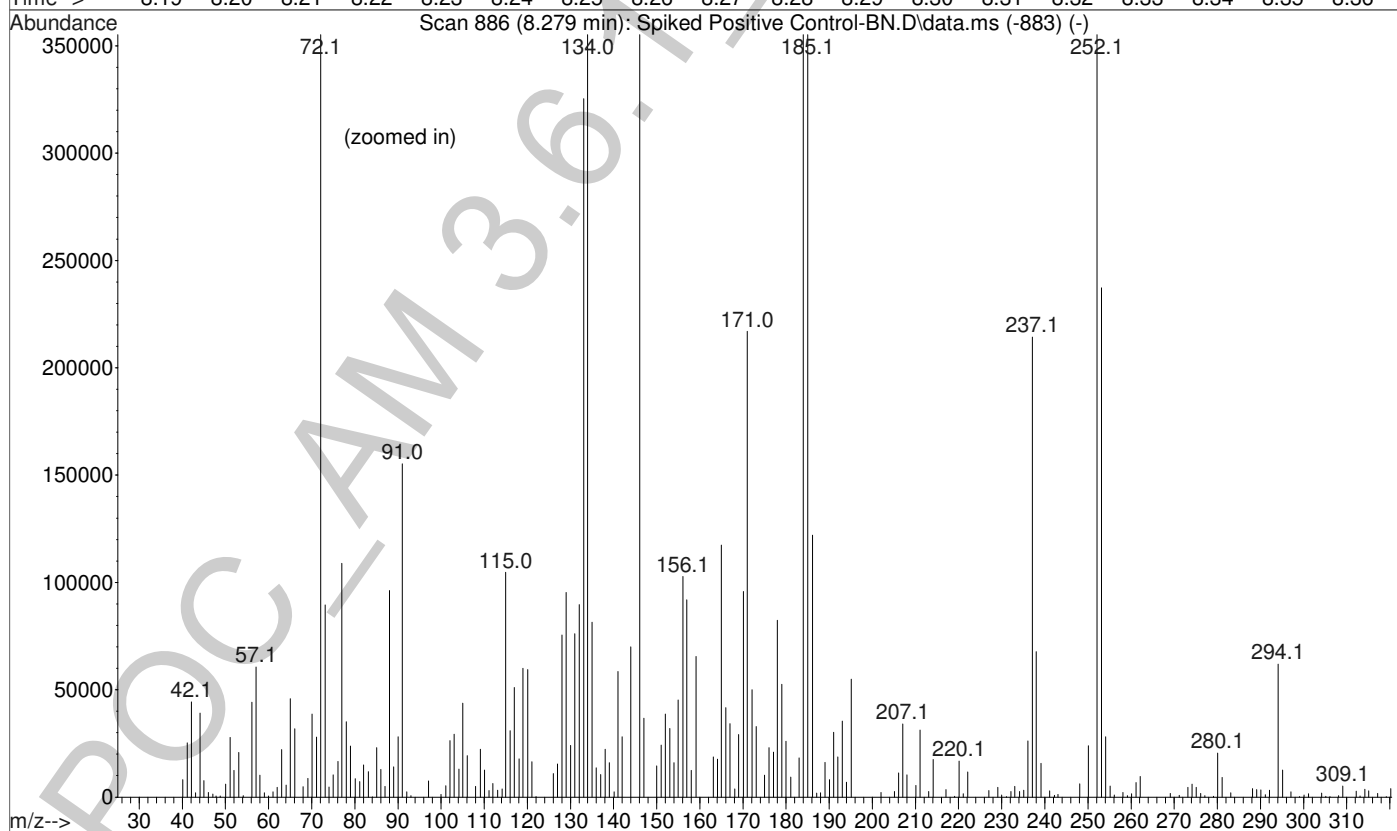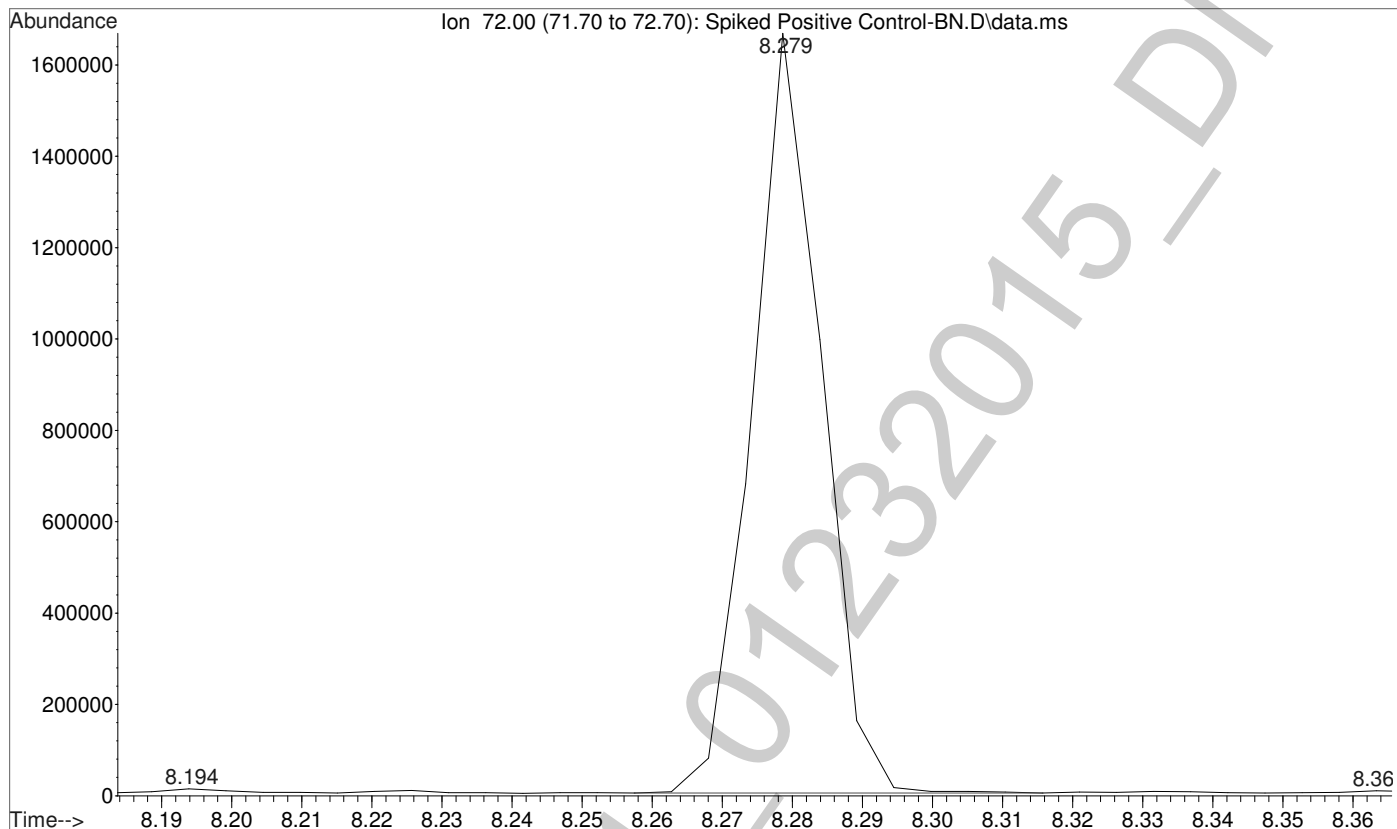



File :C:\gcms\1\data\Blood\012315BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 23 Jan 2015 17:35 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

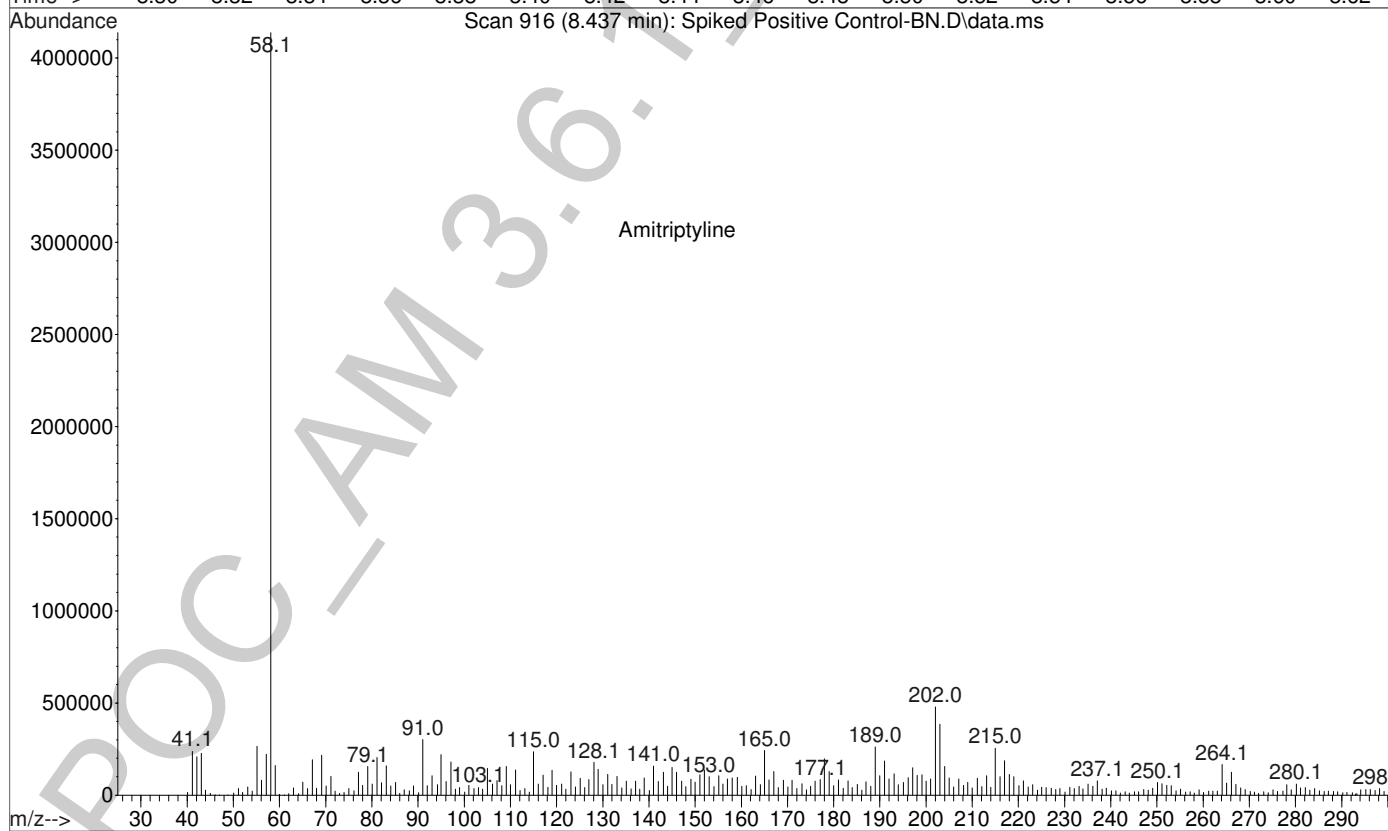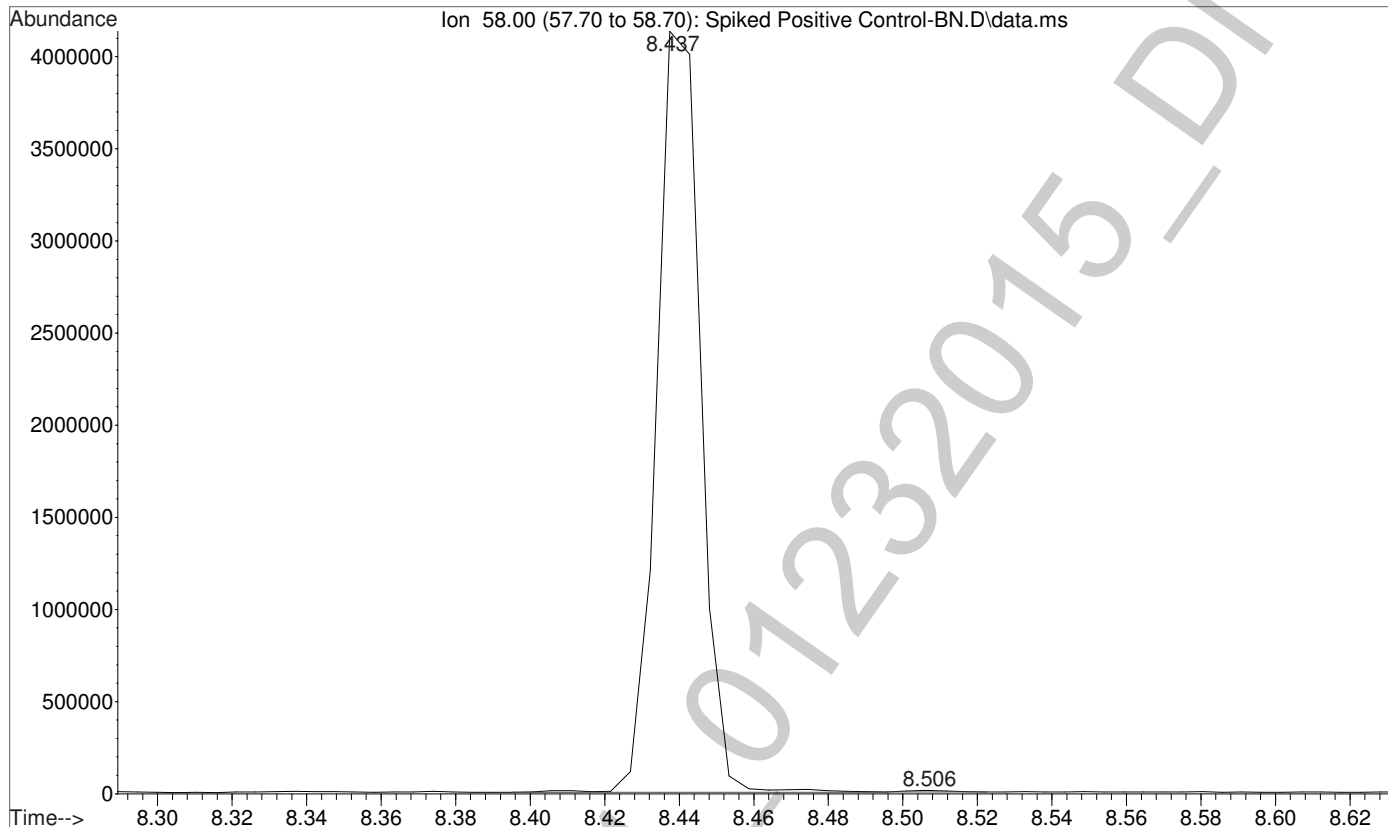



File :C:\gcms\1\data\Blood\012315BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 23 Jan 2015 17:35 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

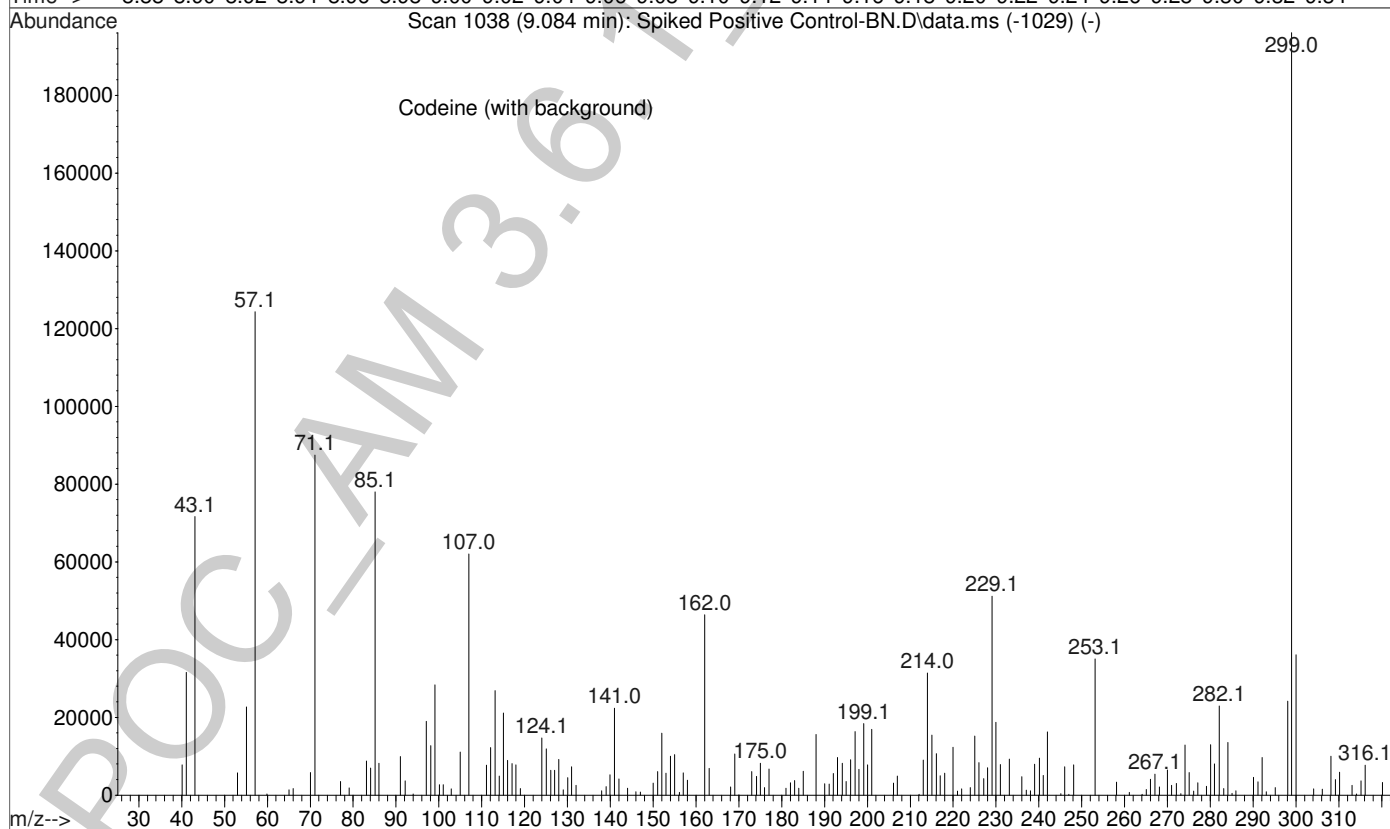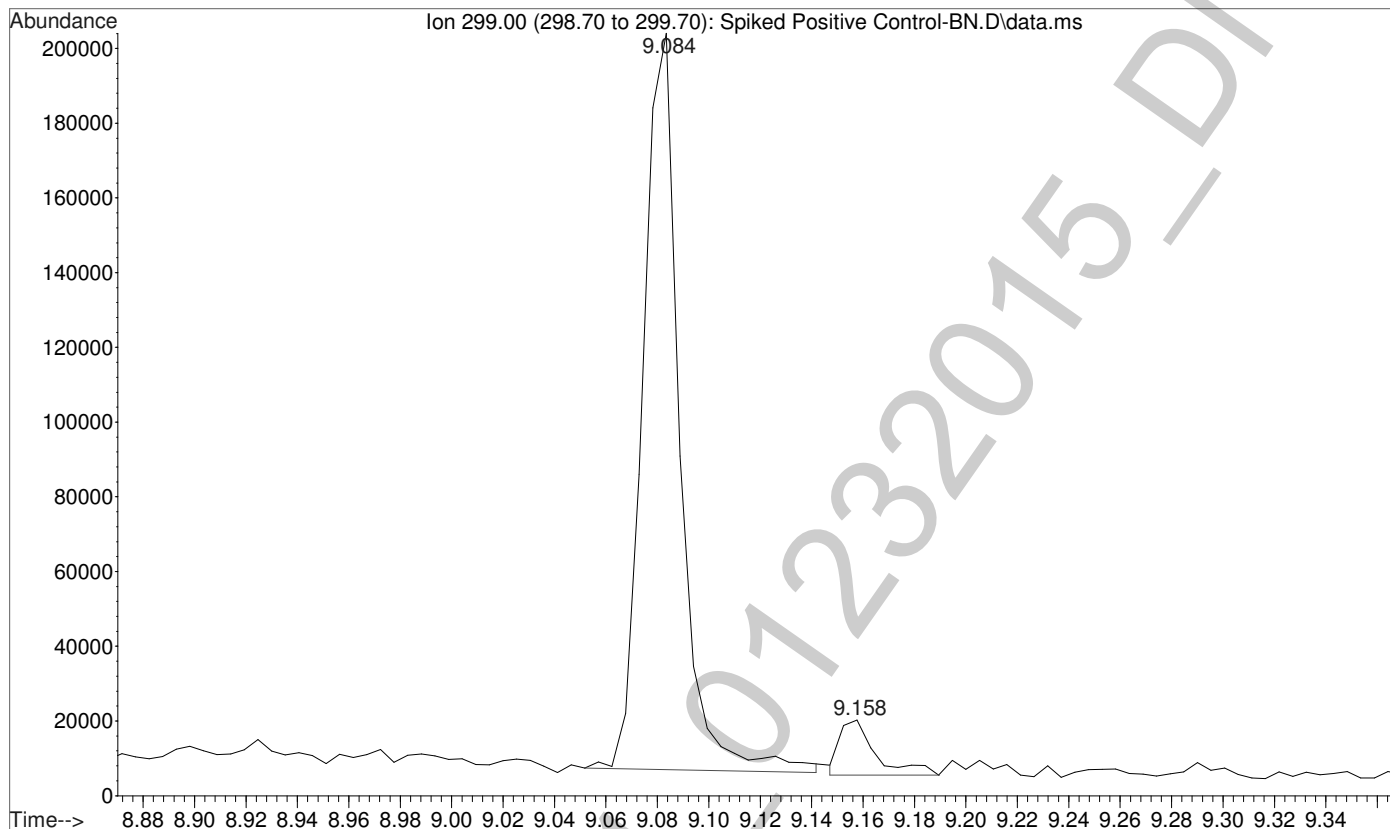

File :C:\gcms\1\data\Blood\012315BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 23 Jan 2015 17:35 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

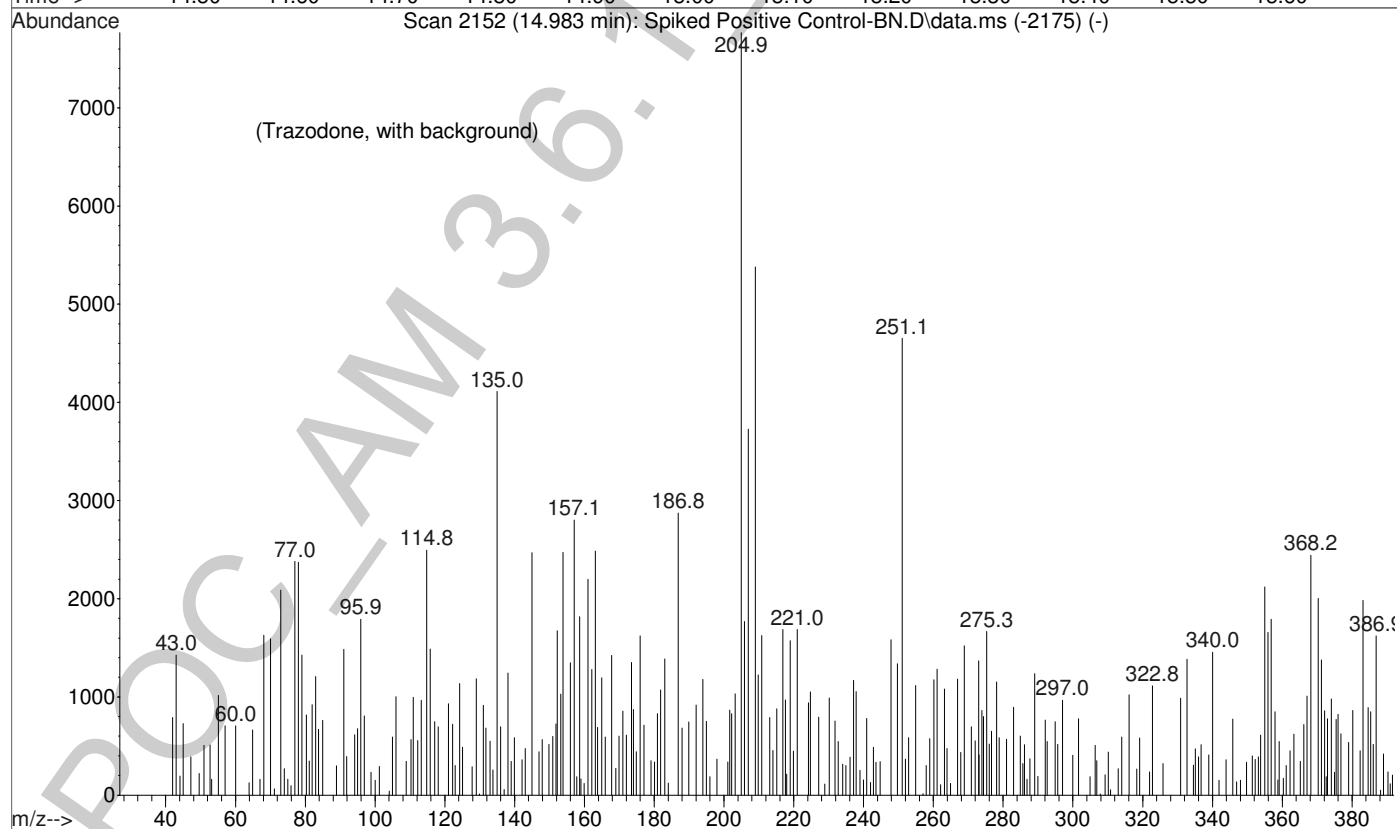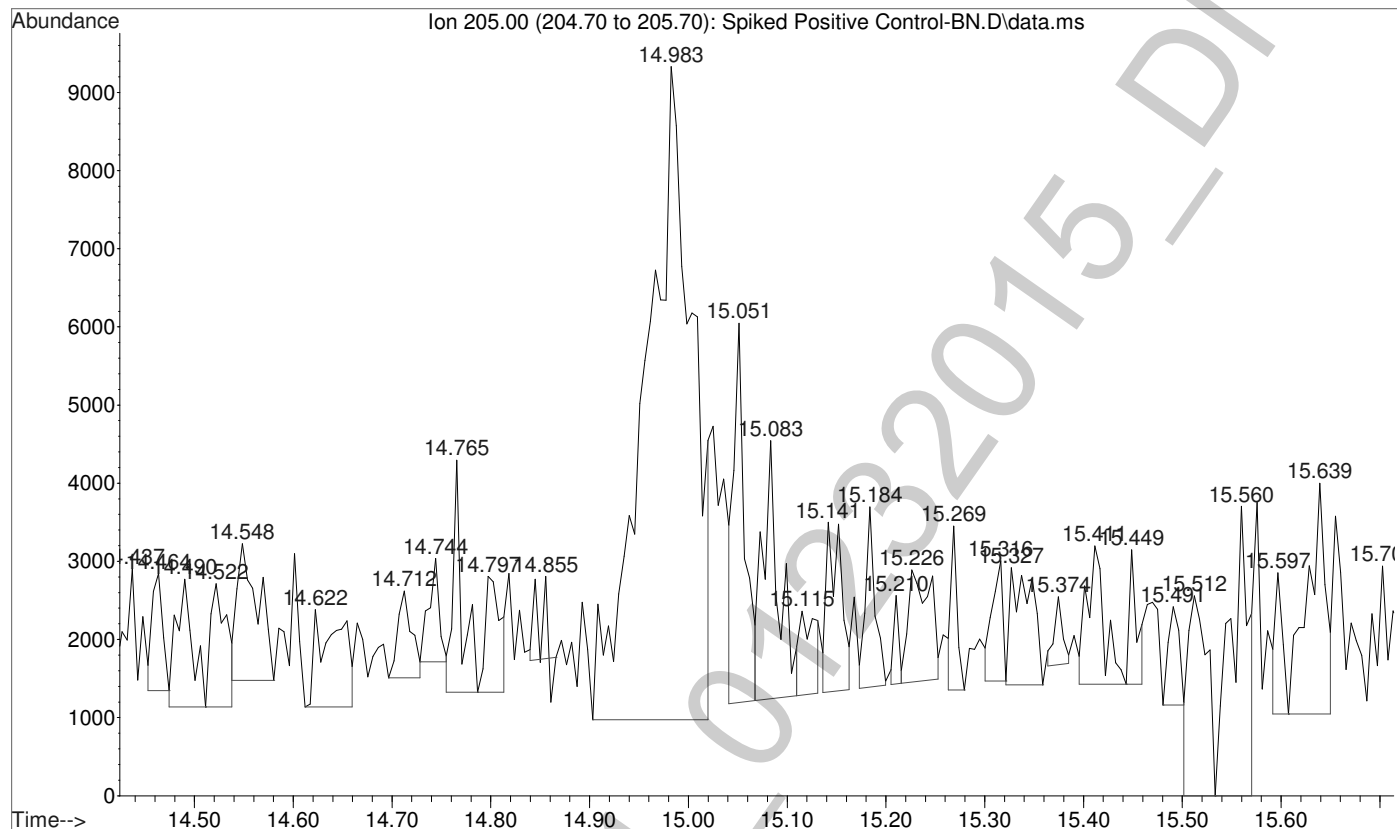

File :C:\gcms\1\data\Blood\012315BN\prbLK2.D
Operator : 5LAB-C01\ISPuser
Acquired : 23 Jan 2015 17:58 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Solvent Blank
Misc Info : Chloroform
Vial Number: 99

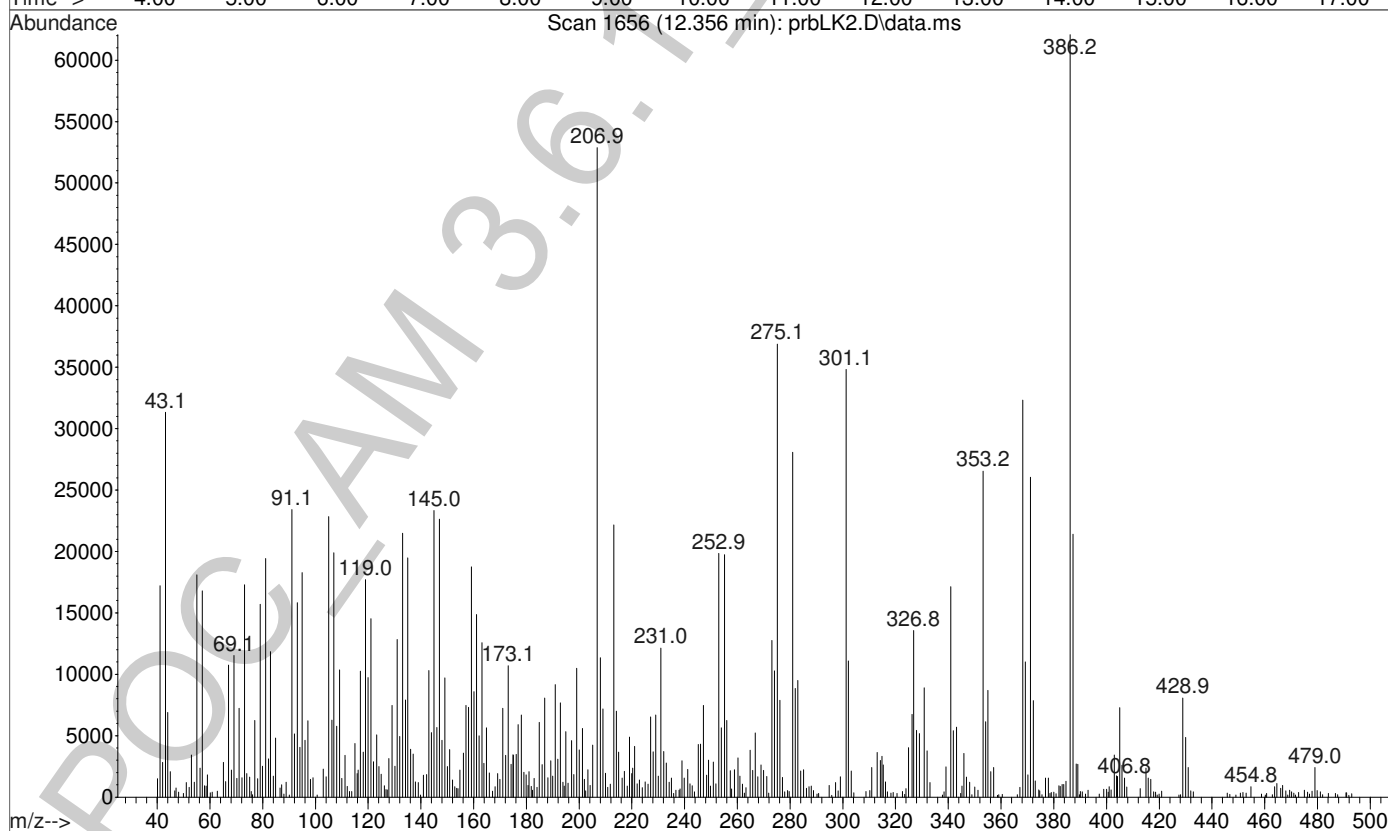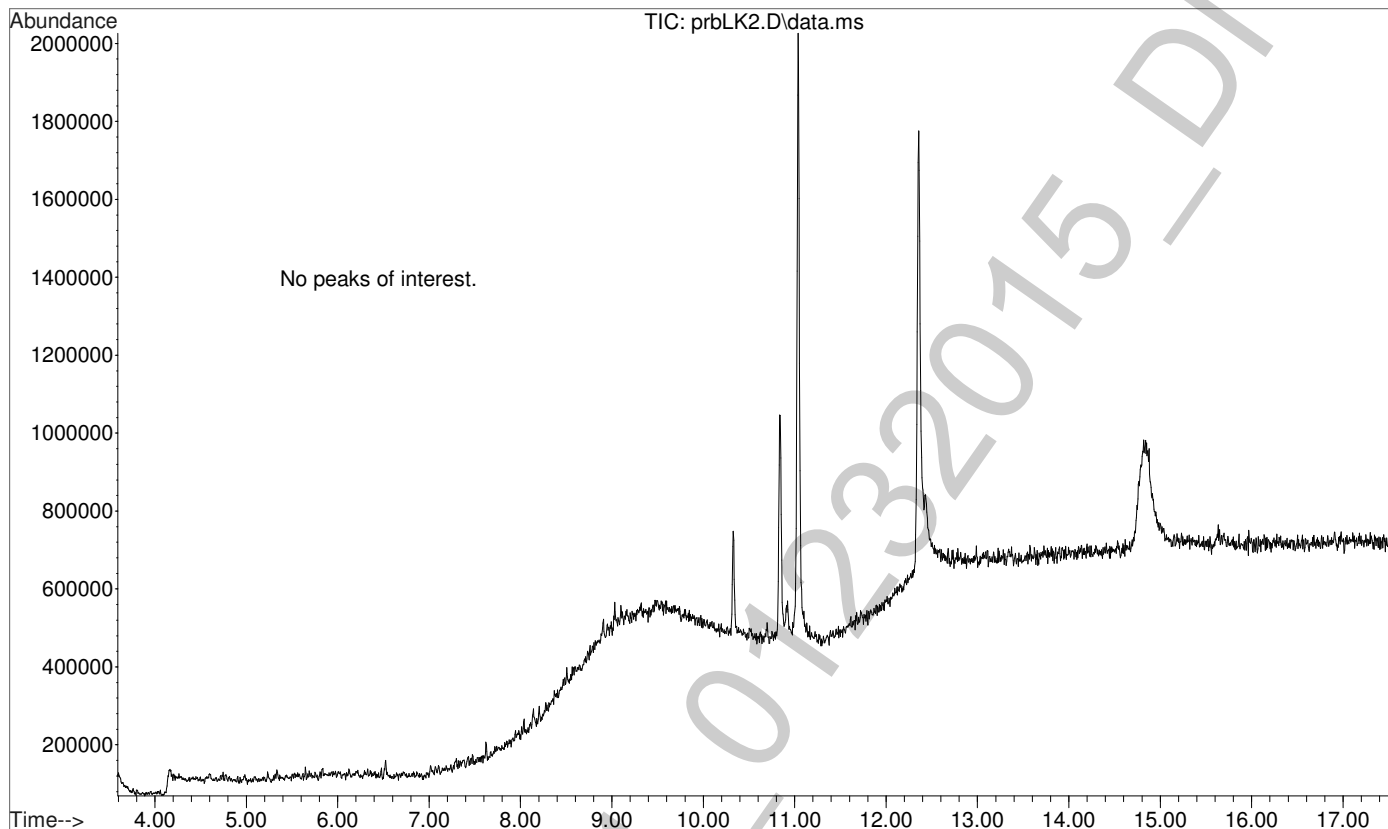

Analytical Method 3.6.1 & 3.6.7 QA Check List

Run Start Date: 01/23/15

Analyst: DND

(Long GC/MS temperature program)

Positive Control Compound List

- Methamphetamine
- Nicotine
- Meperidine
- Caffeine
- Diphenhydramine
- Lidocaine
- PCP
- Methadone
- Amitriptyline
- Codeine
- Trazodone

Internal Standards


- Benzphetamine
- Papaverine

Optional back extraction **not** performed.
Samples reconstituted in methanol.





POC_AM3.6.1_01232015_DND

File :C:\gcms\1\data\Blood\012315BN\Reinjection Longer GC Method\N
... egative Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 23 Jan 2015 18:55 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Negative Control - Utak Lot B0130
Misc Info : Analytical Method 3.6.1


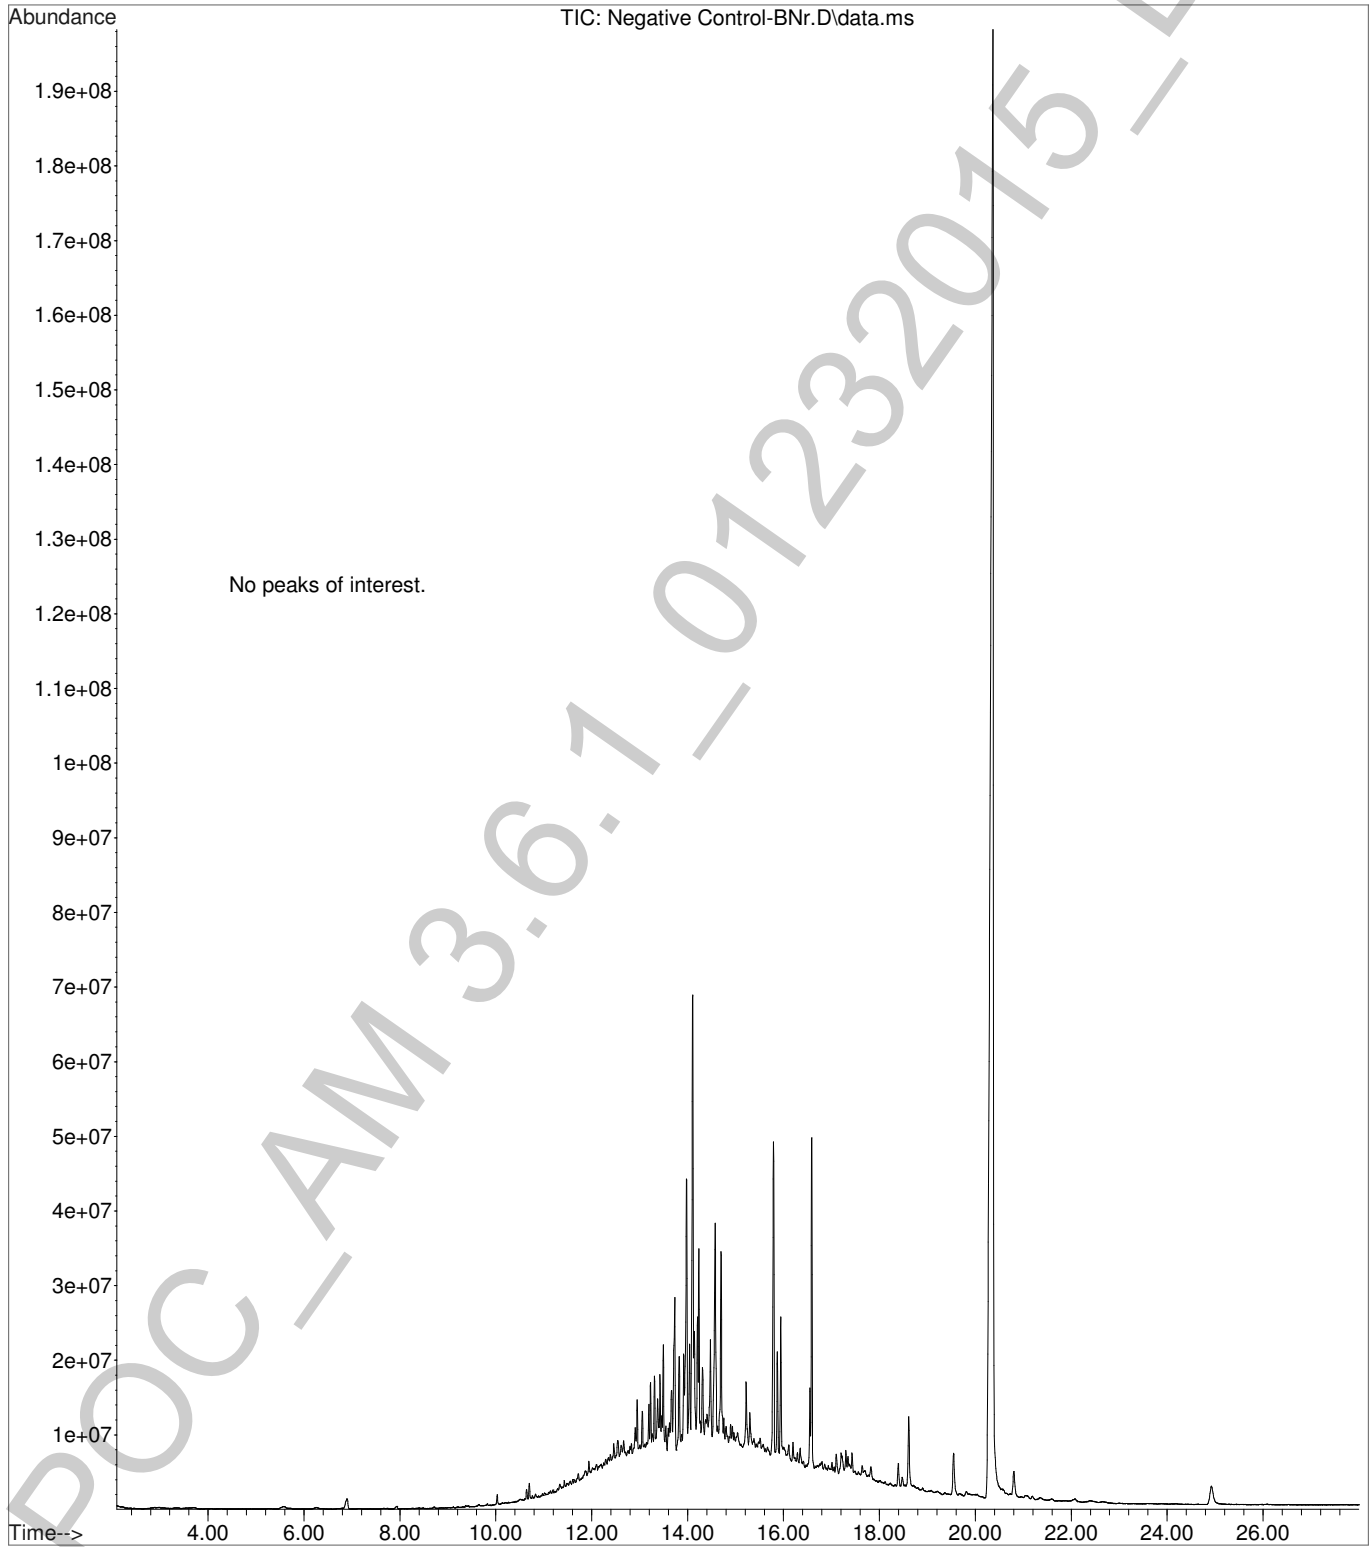


File :C:\gcms\1\data\Blood\012315BN\Reinjection Longer GC Method\N
... egative Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 23 Jan 2015 18:55 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Negative Control - Utak Lot B0130
Misc Info : Analytical Method 3.6.1

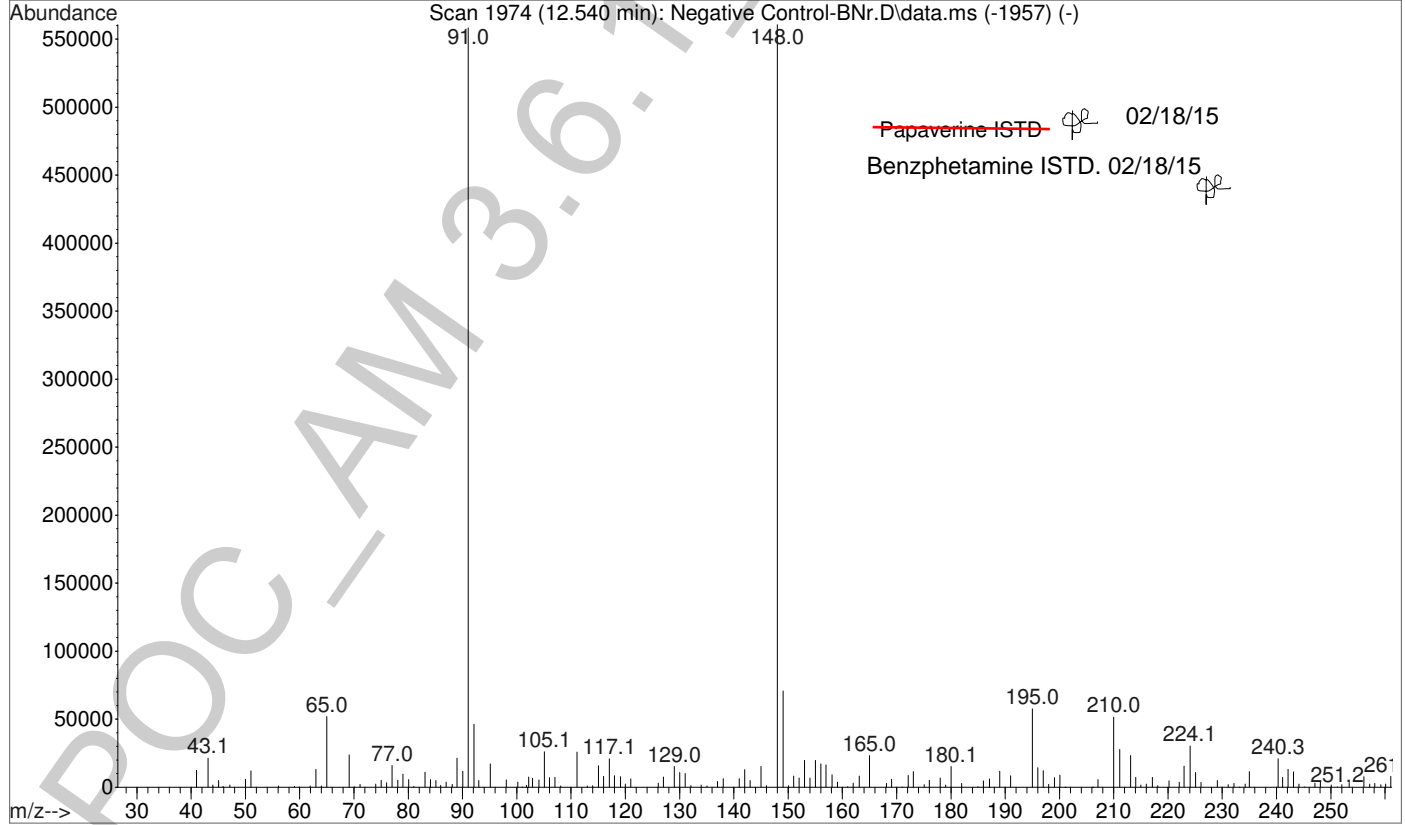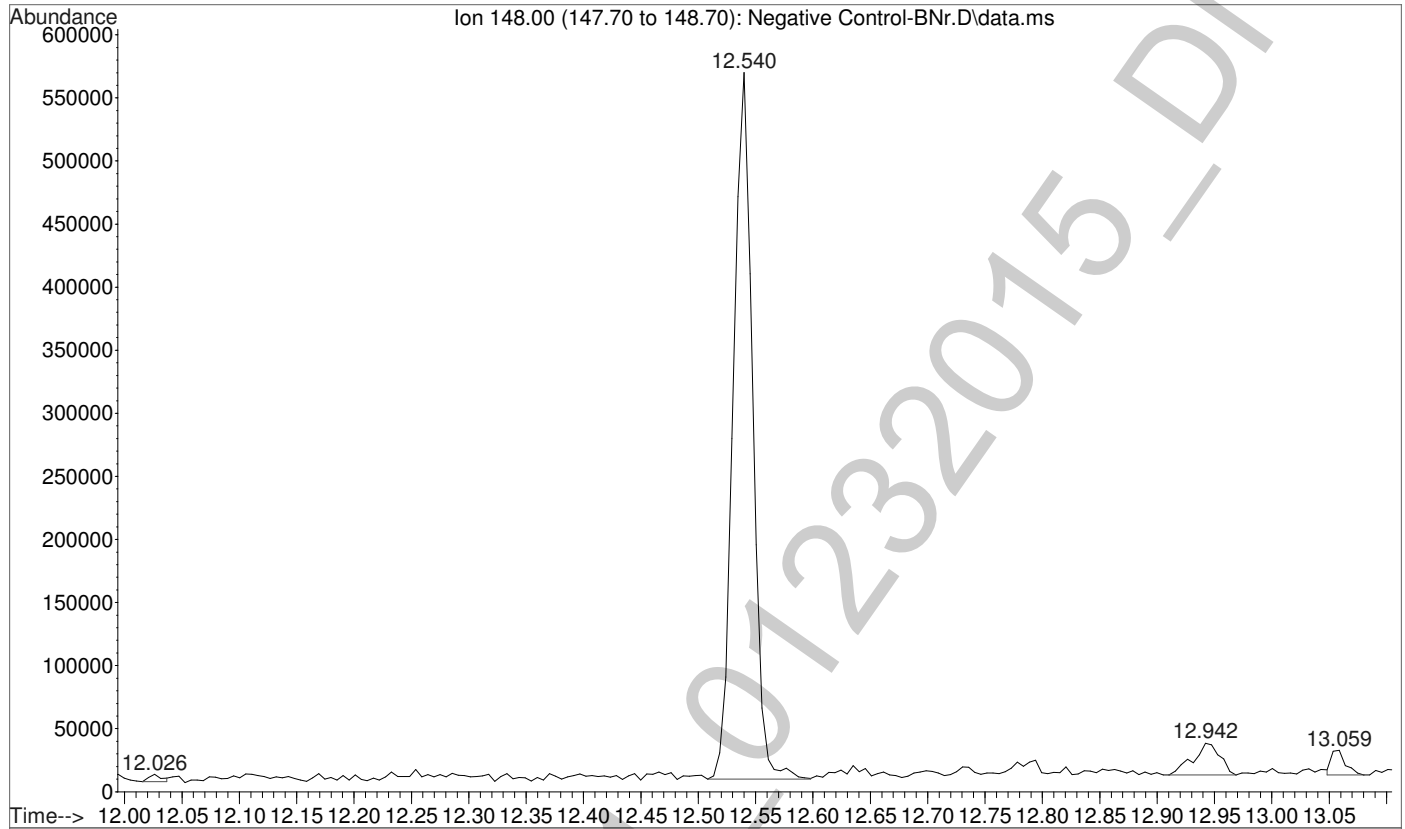


~~Papaverine~~ ISTD 02/18/15
Benzphetamine ISTD. 02/18/15



File :C:\gcms\1\data\Blood\012315BN\Reinjection Longer GC Method\N
... egative Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 23 Jan 2015 18:55 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Negative Control - Utak Lot B0130
Misc Info : Analytical Method 3.6.1

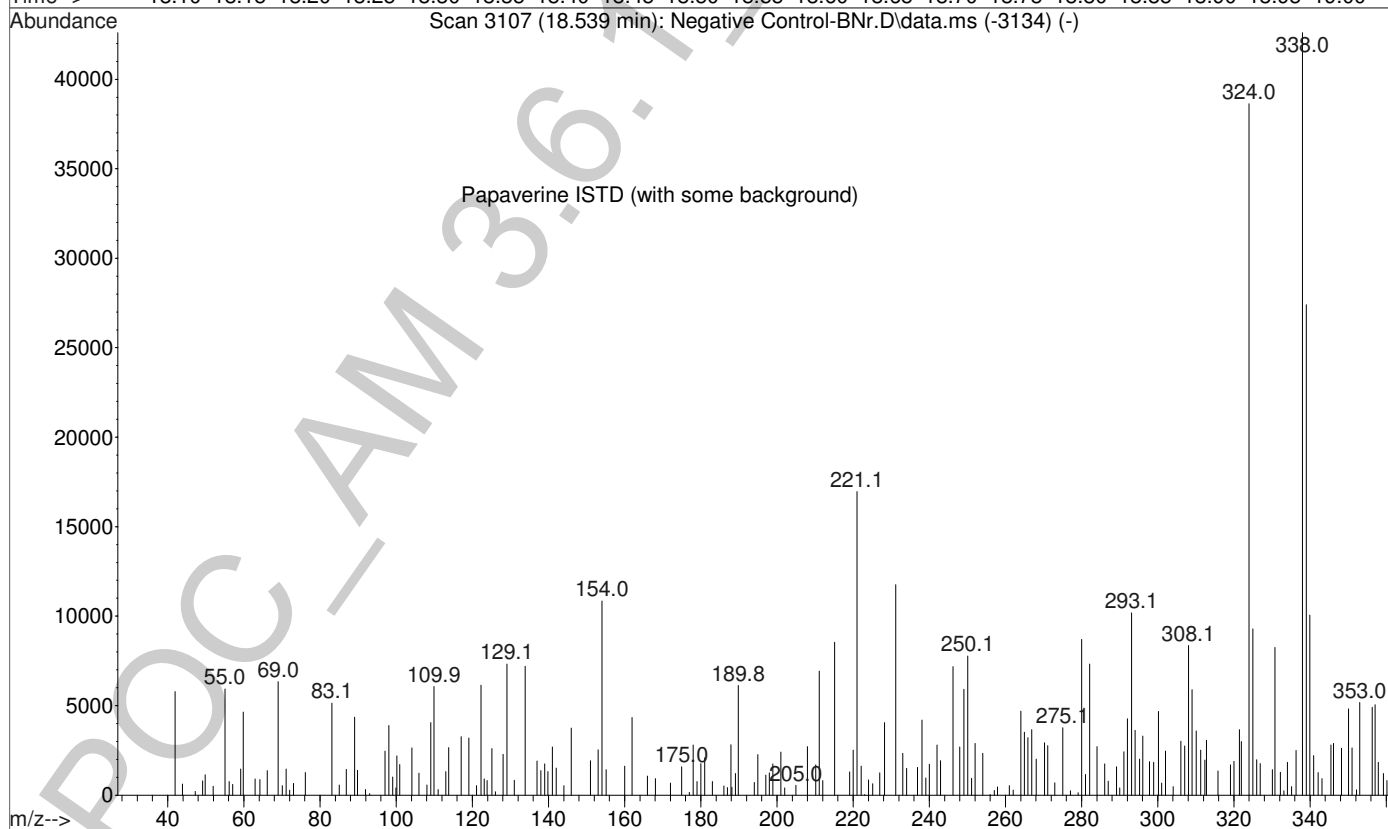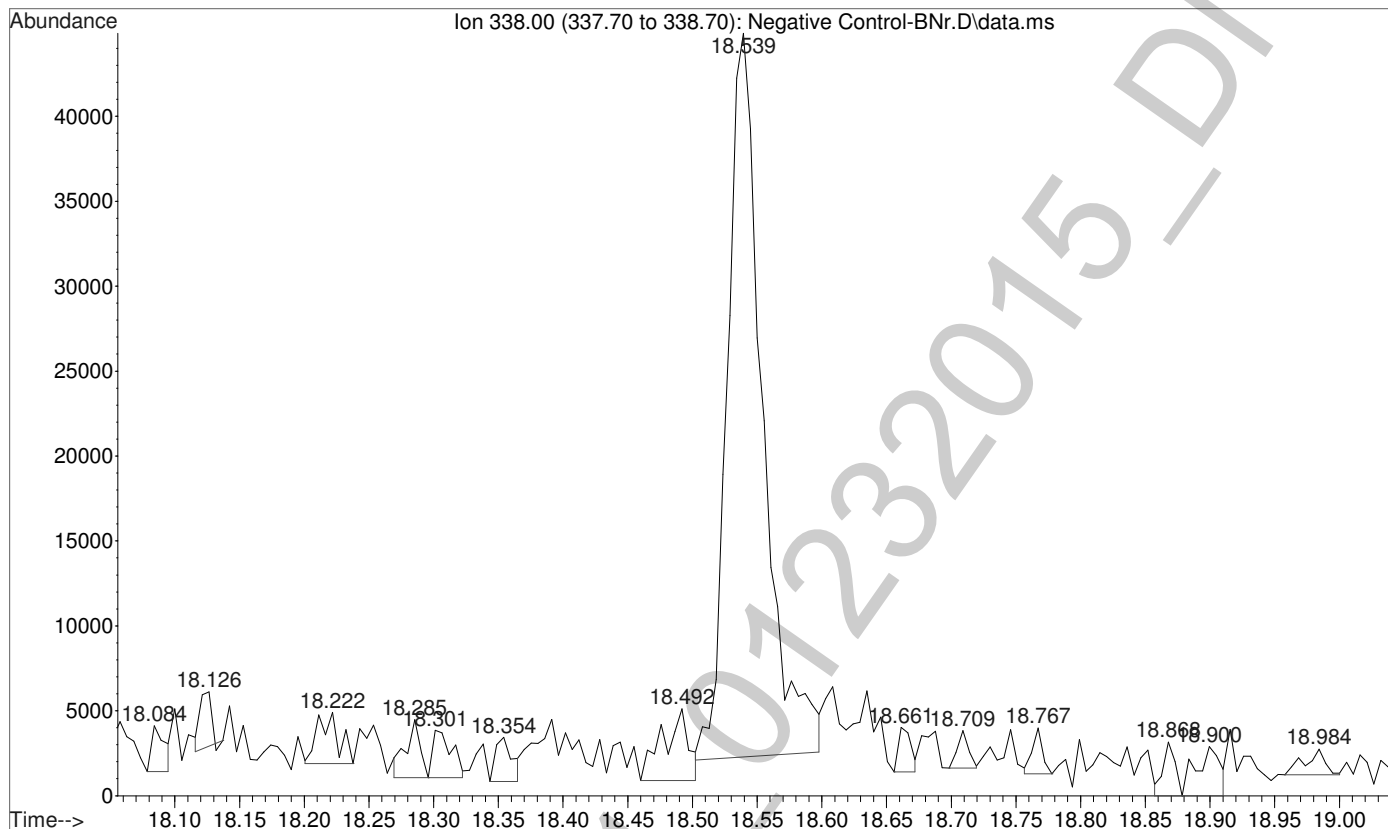



File :C:\gcms\1\data\Blood\012315BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 23 Jan 2015 19:29 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

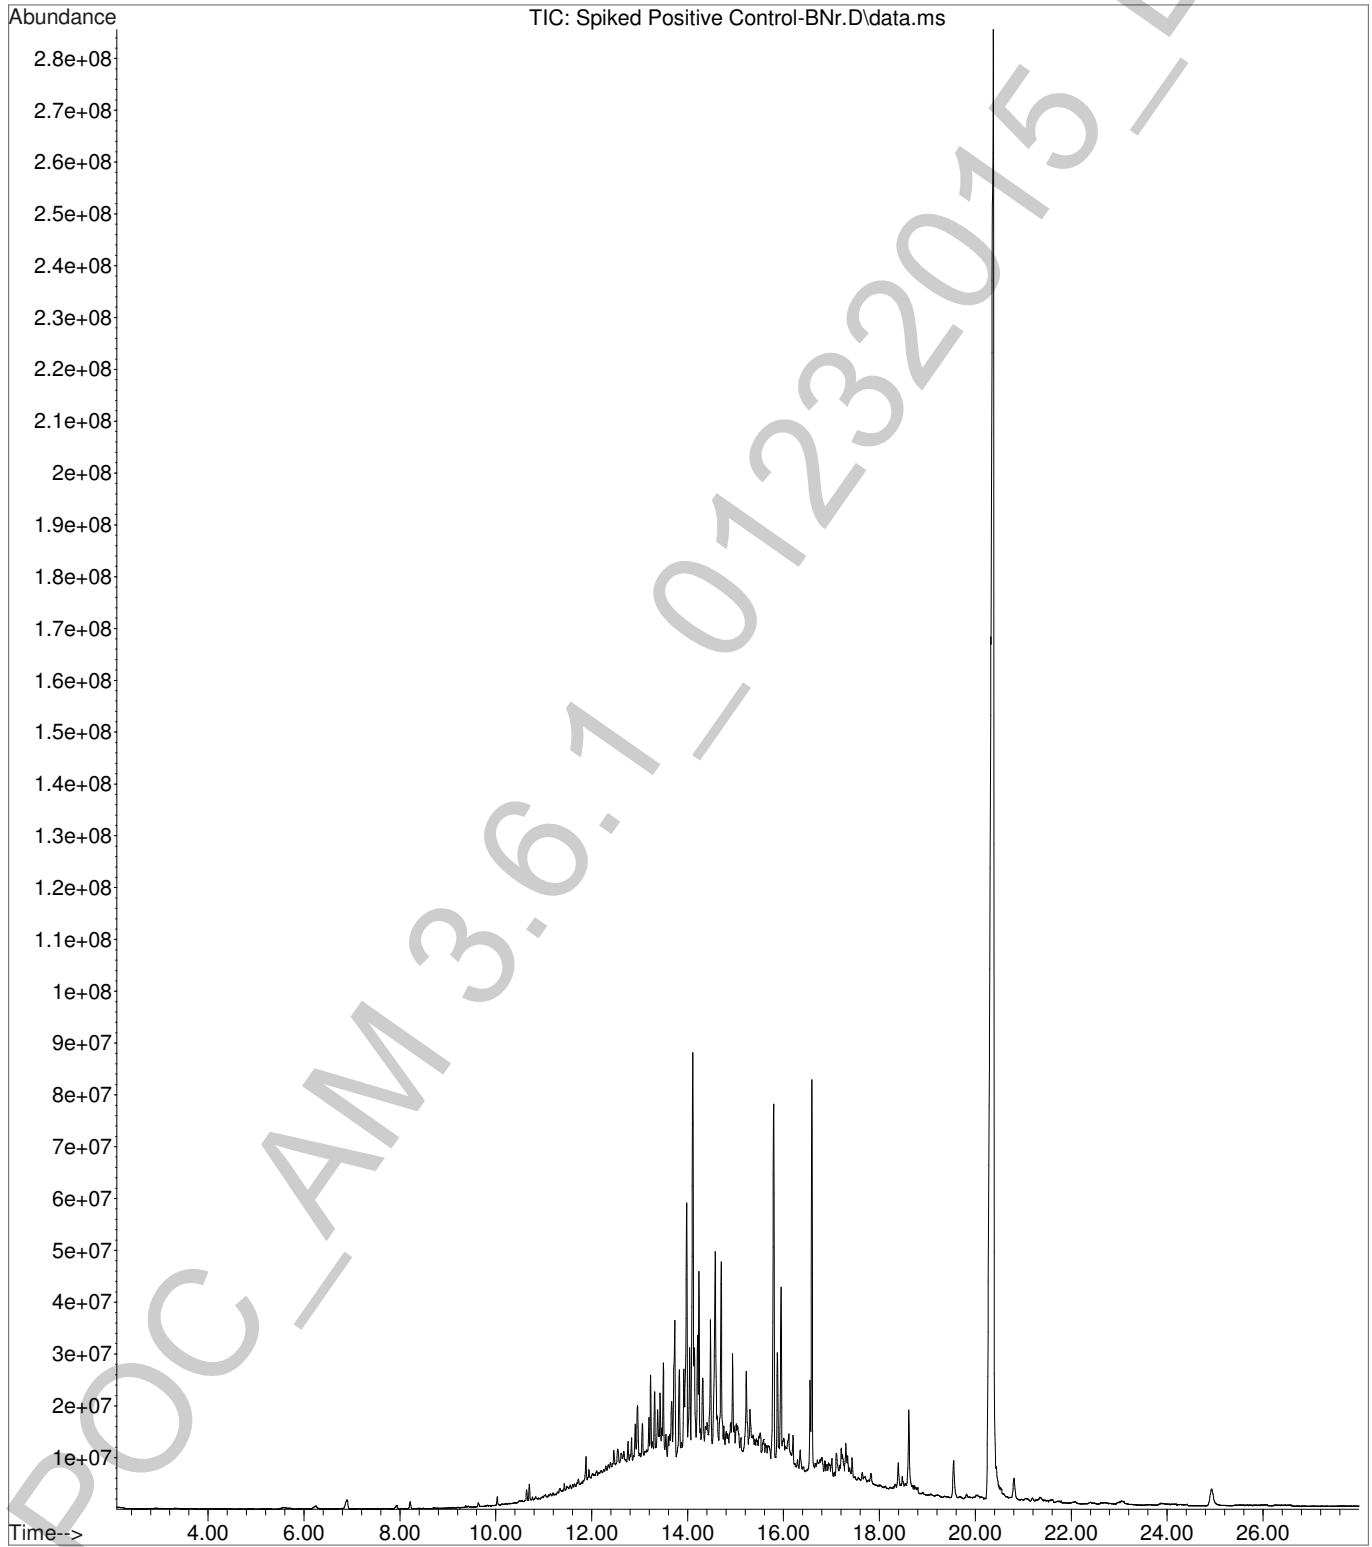



File :C:\gcms\1\data\Blood\012315BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 23 Jan 2015 19:29 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

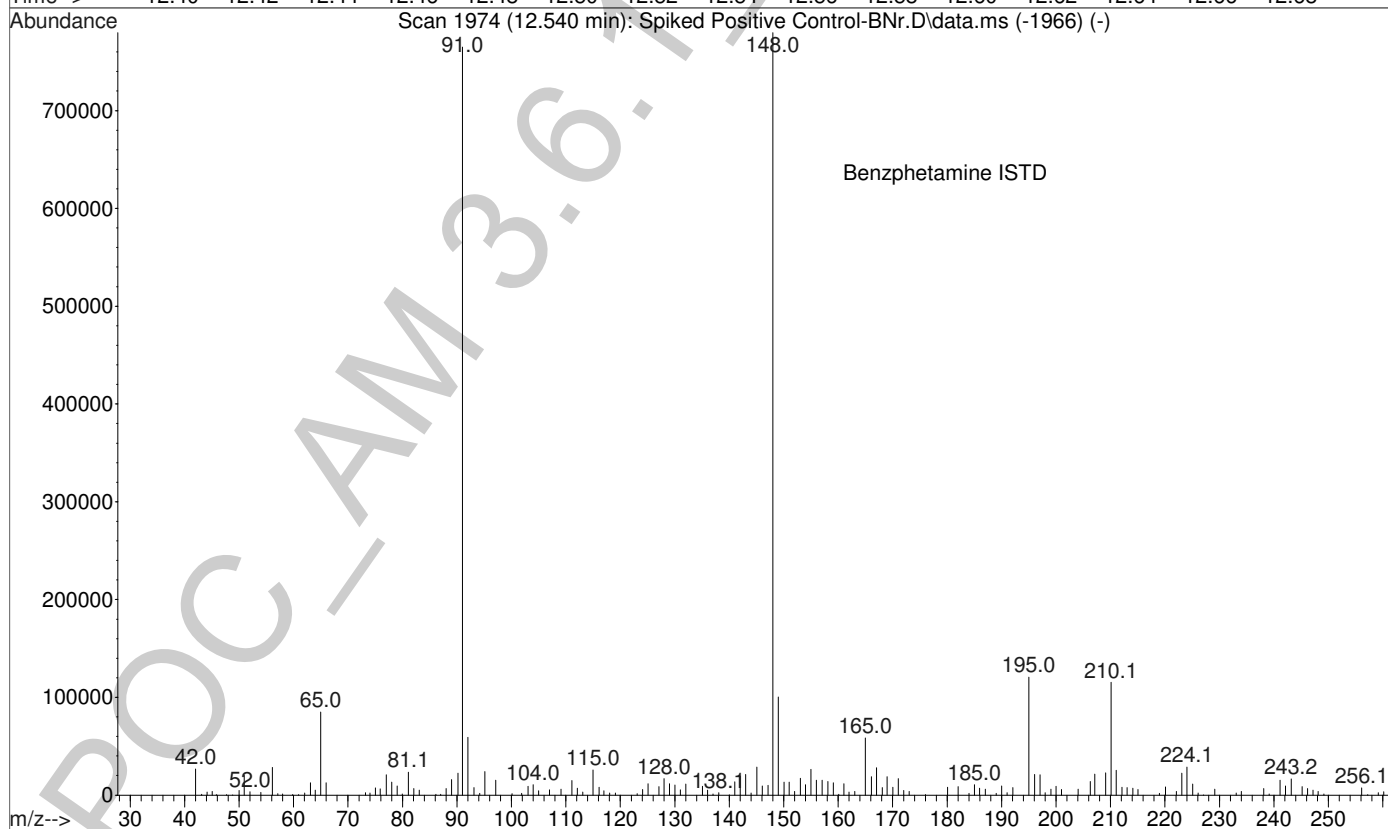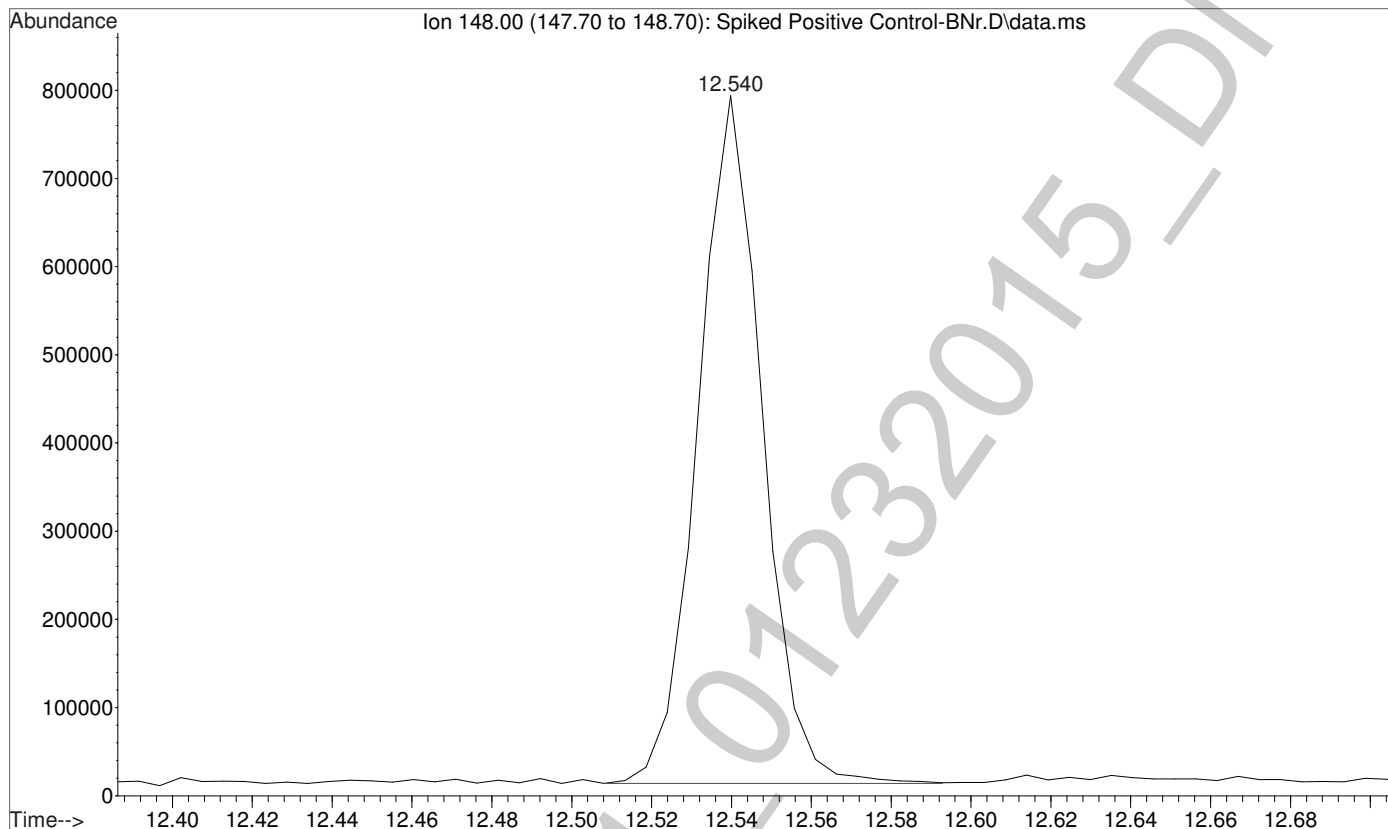



File :C:\gcms\1\data\Blood\012315BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 23 Jan 2015 19:29 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

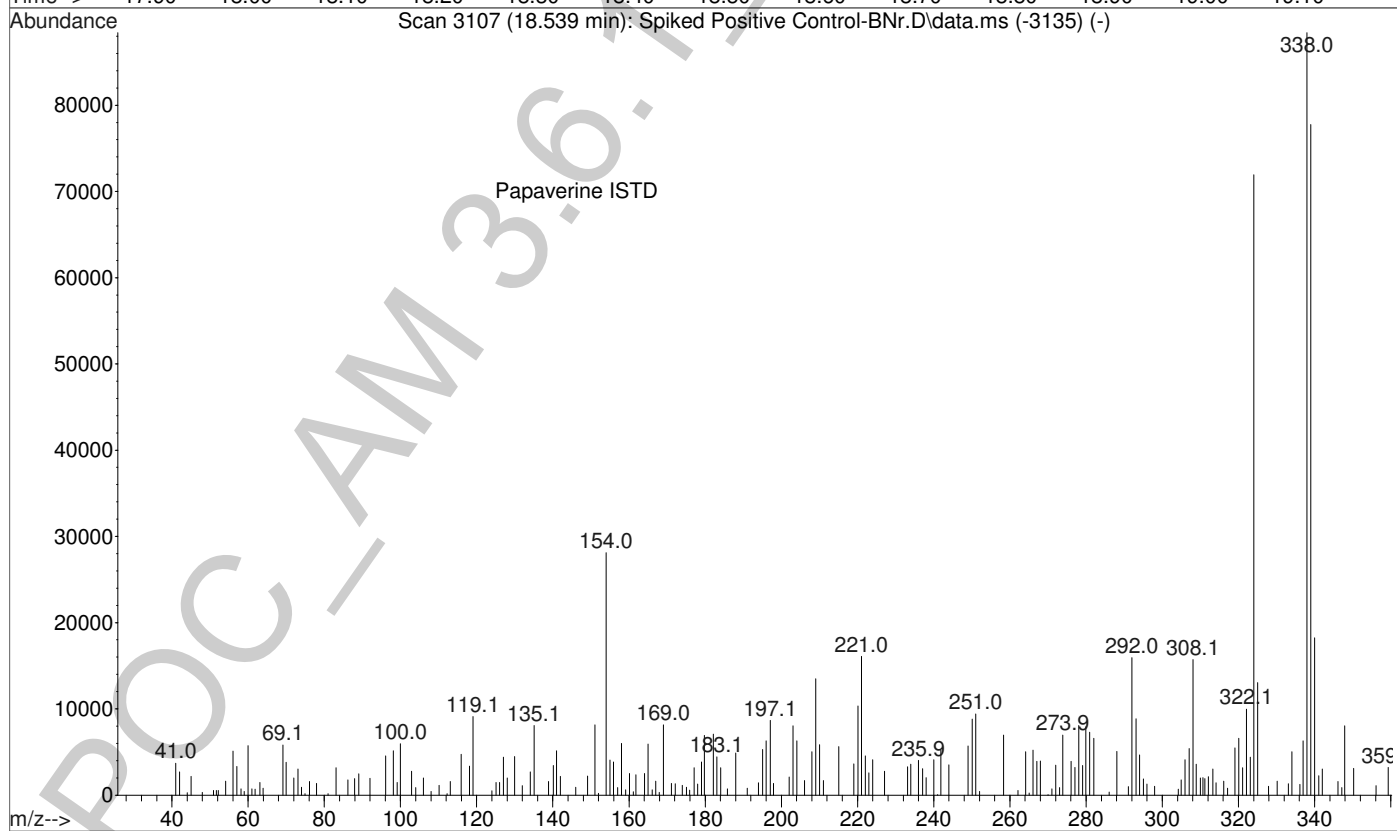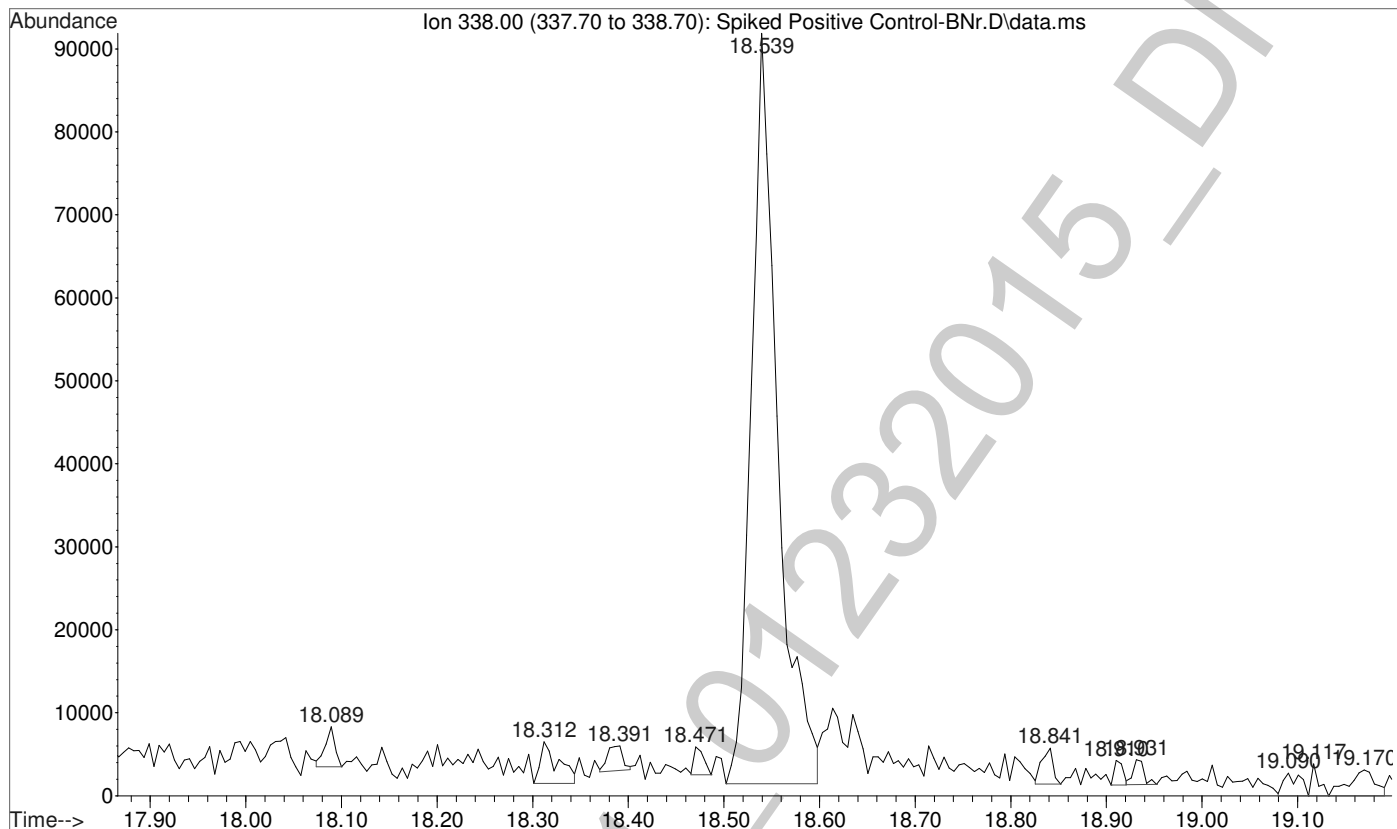



File :C:\gcms\1\data\Blood\012315BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 23 Jan 2015 19:29 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

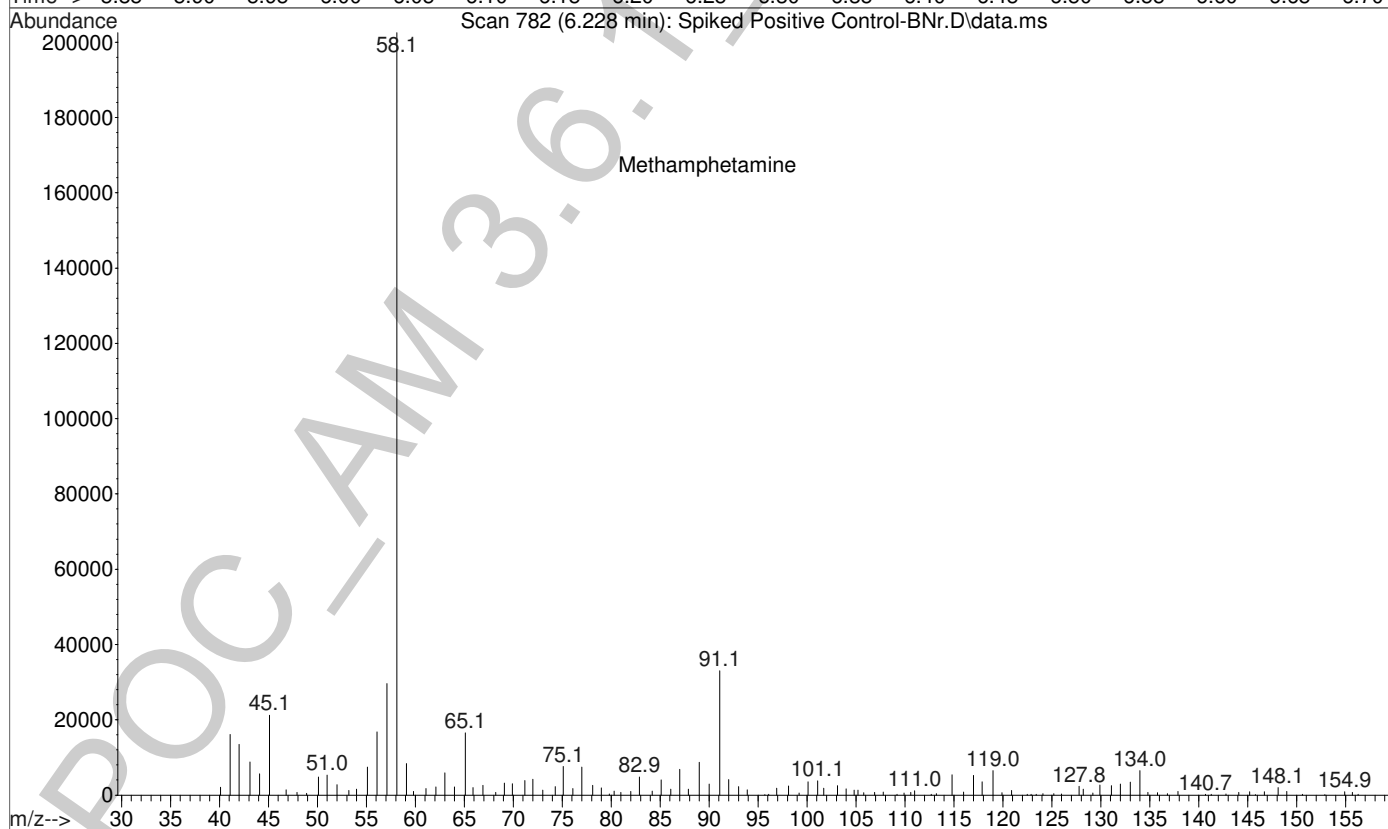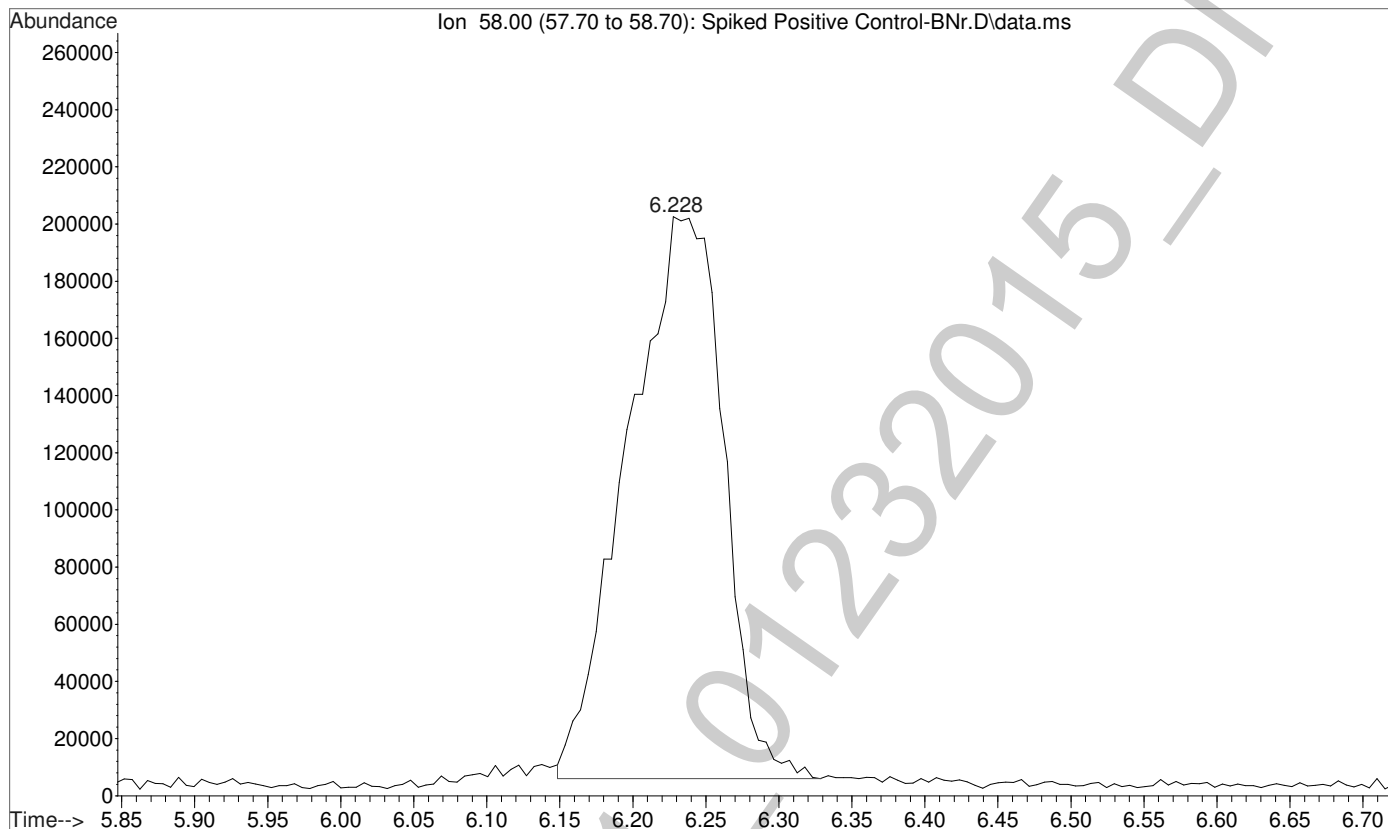



File :C:\gcms\1\data\Blood\012315BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 23 Jan 2015 19:29 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

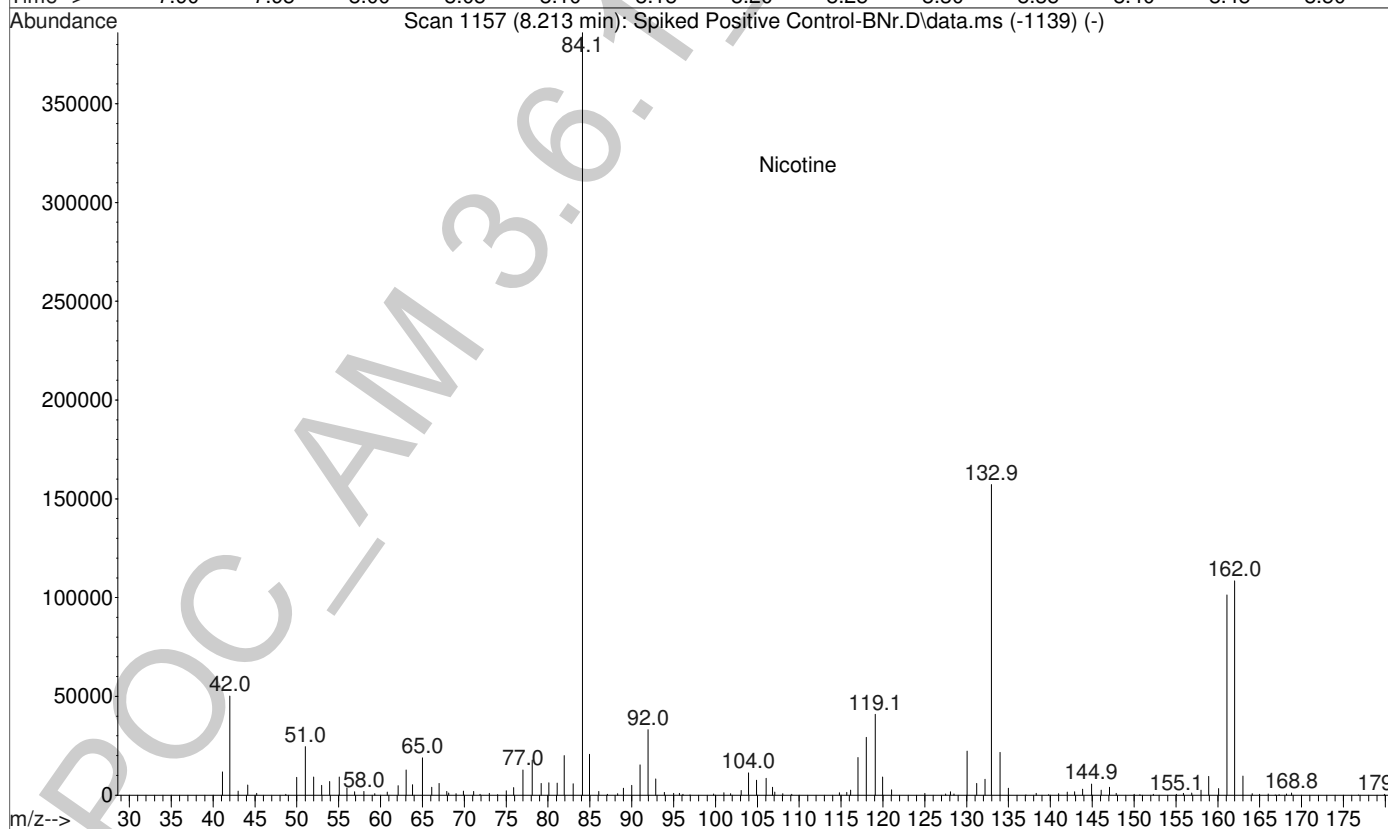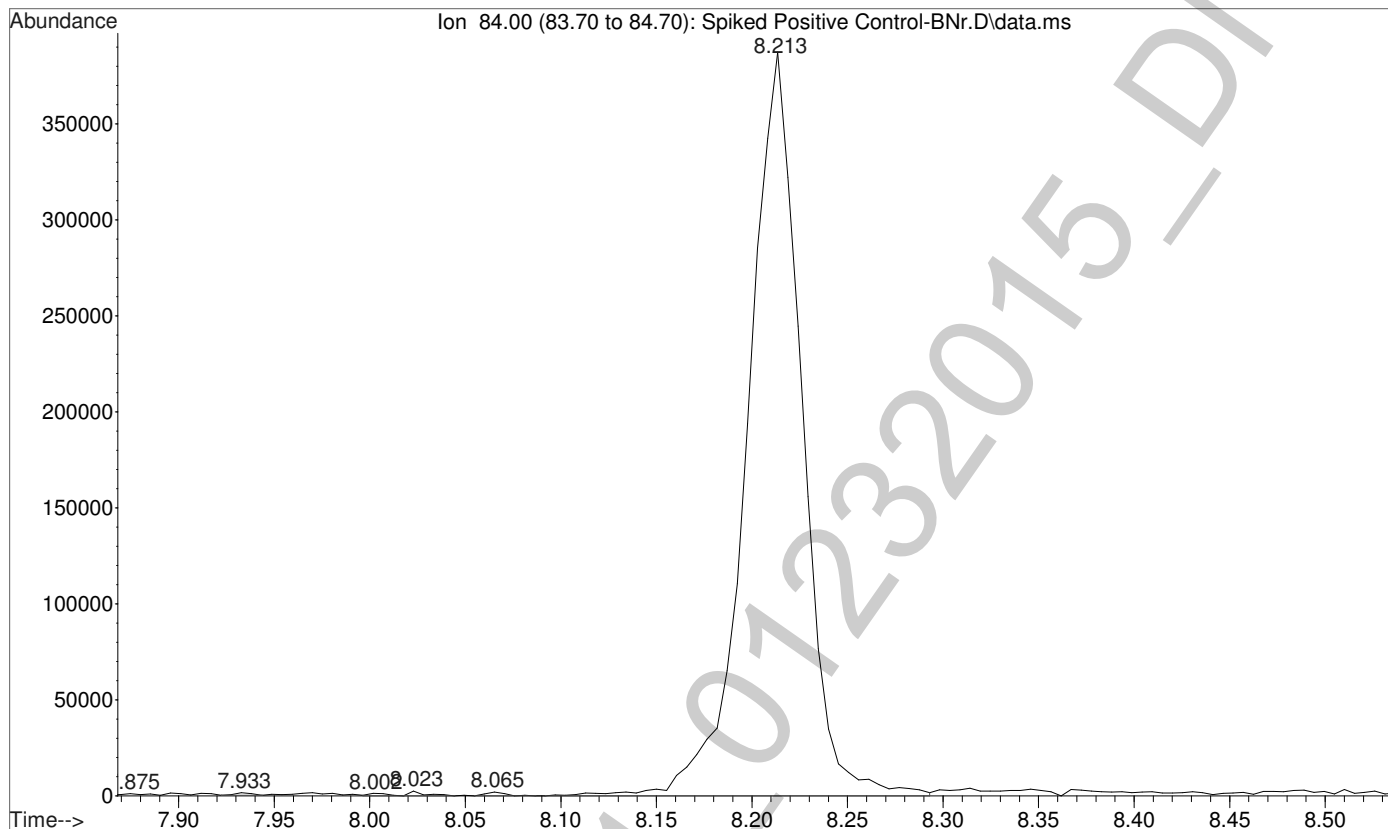



File :C:\gcms\1\data\Blood\012315BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 23 Jan 2015 19:29 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

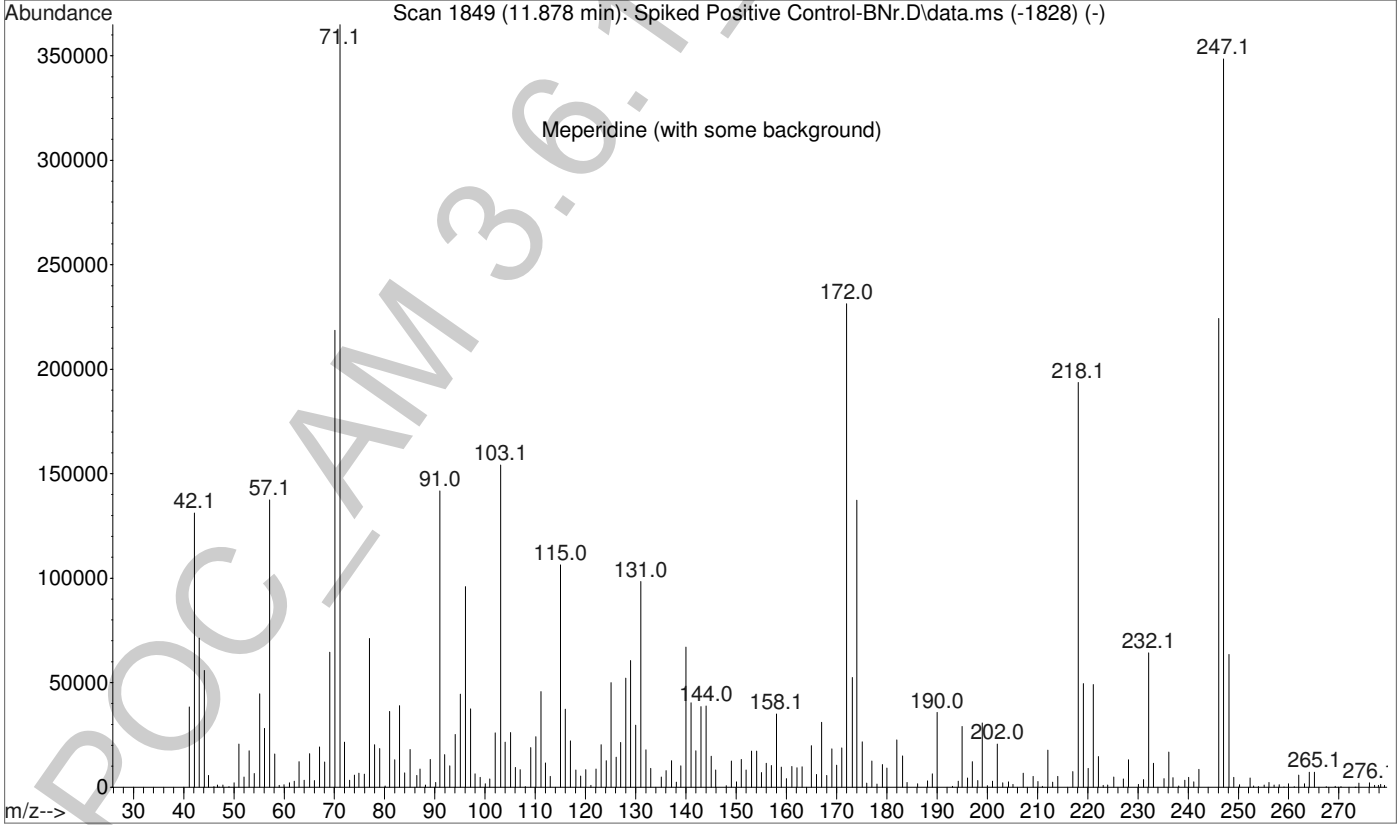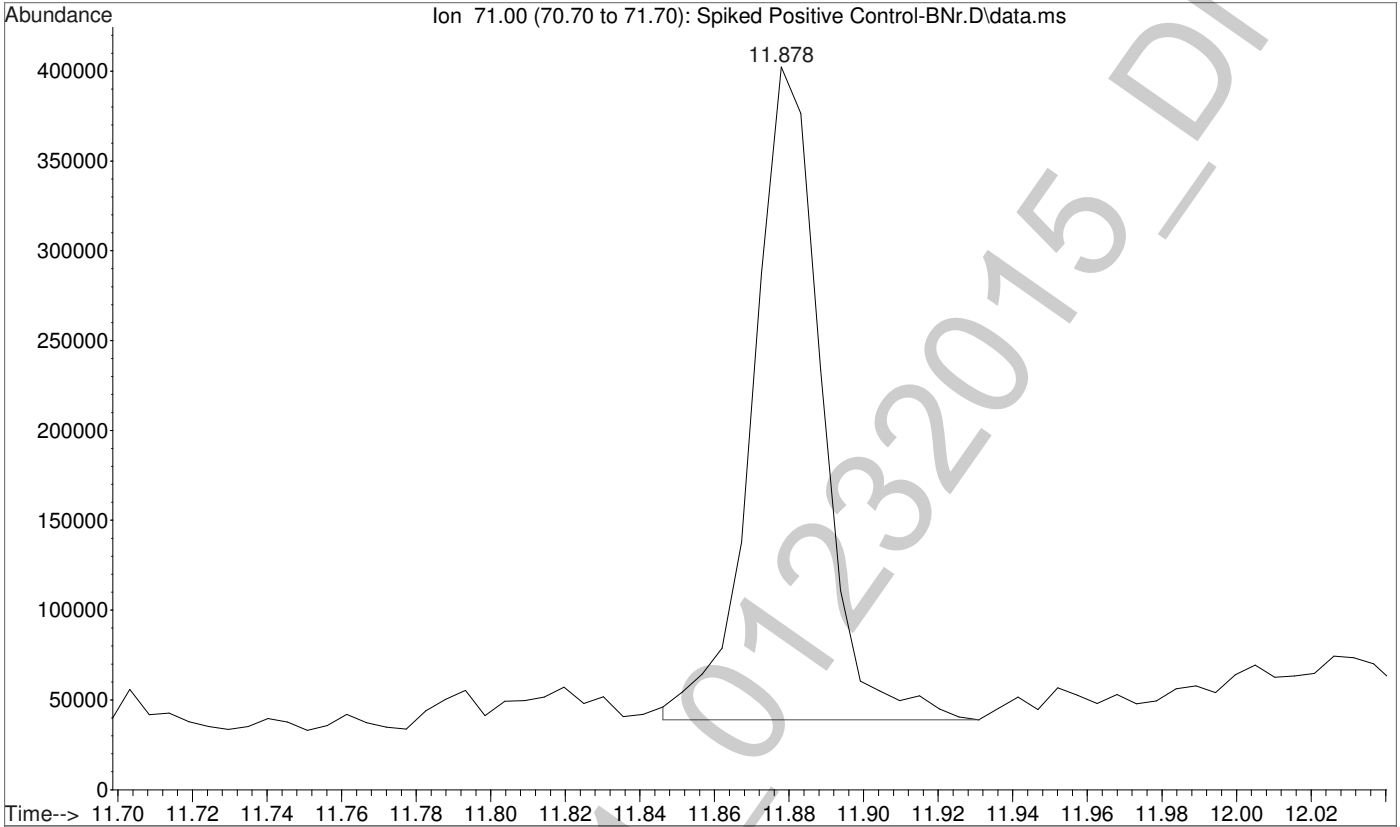



File :C:\gcms\1\data\Blood\012315BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 23 Jan 2015 19:29 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

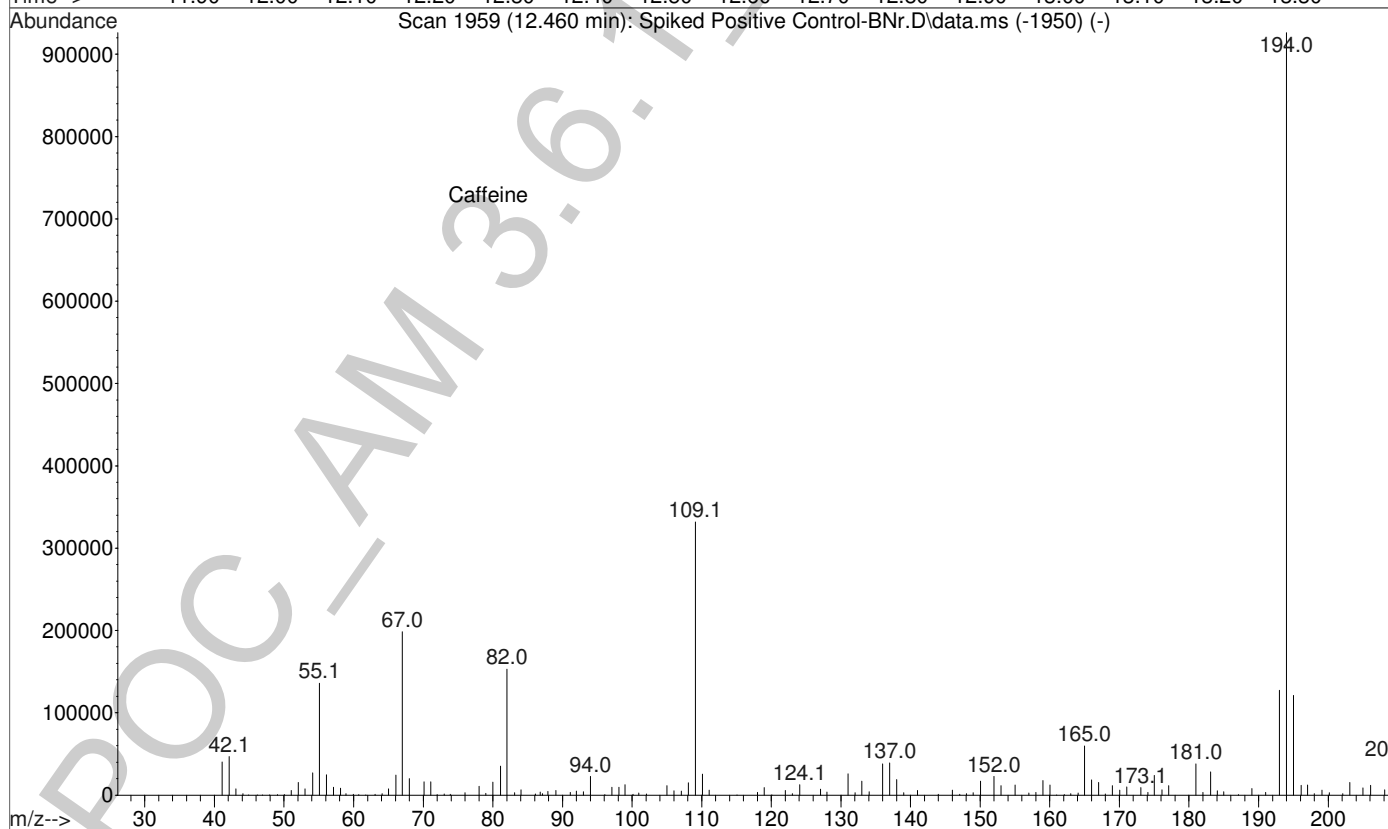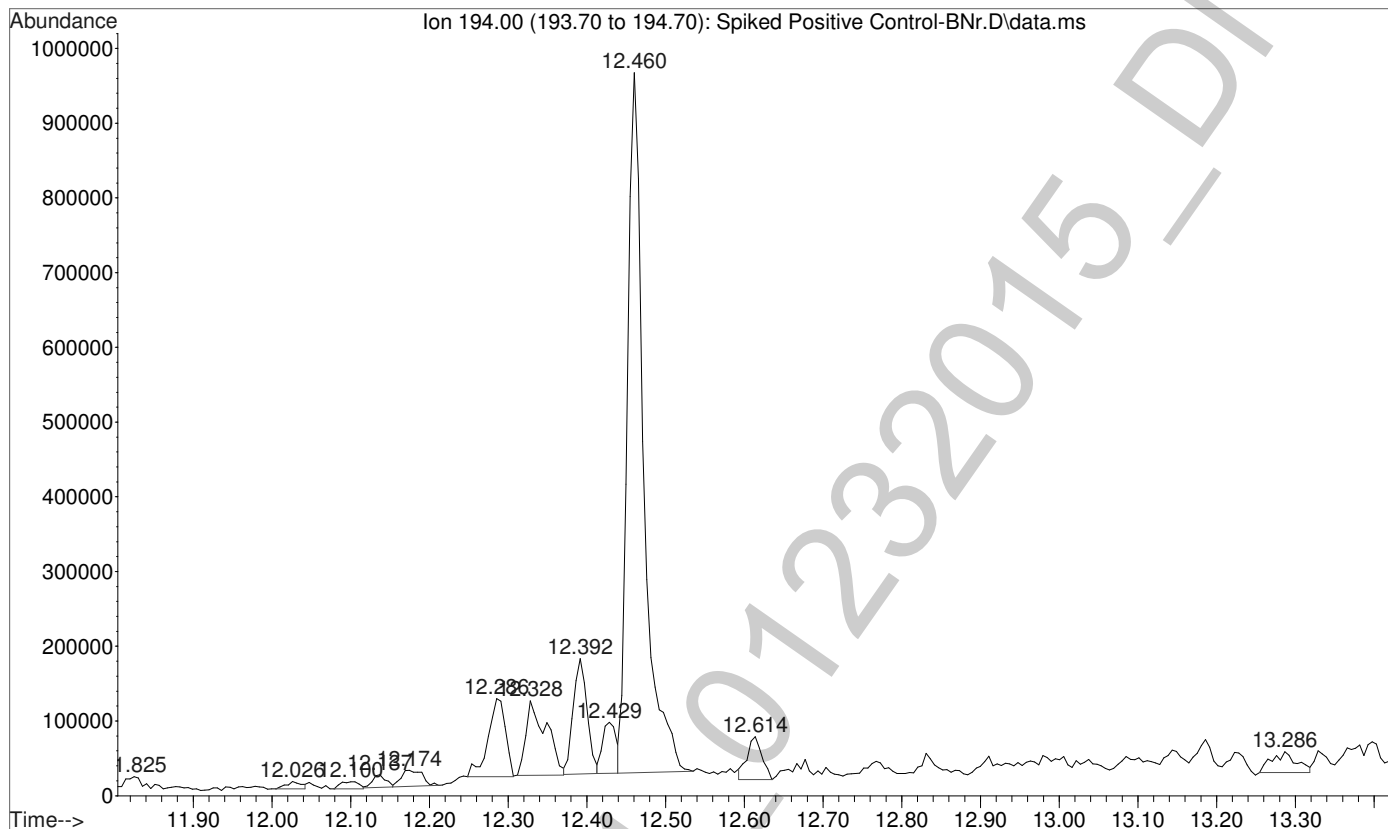



File :C:\gcms\1\data\Blood\012315BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 23 Jan 2015 19:29 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

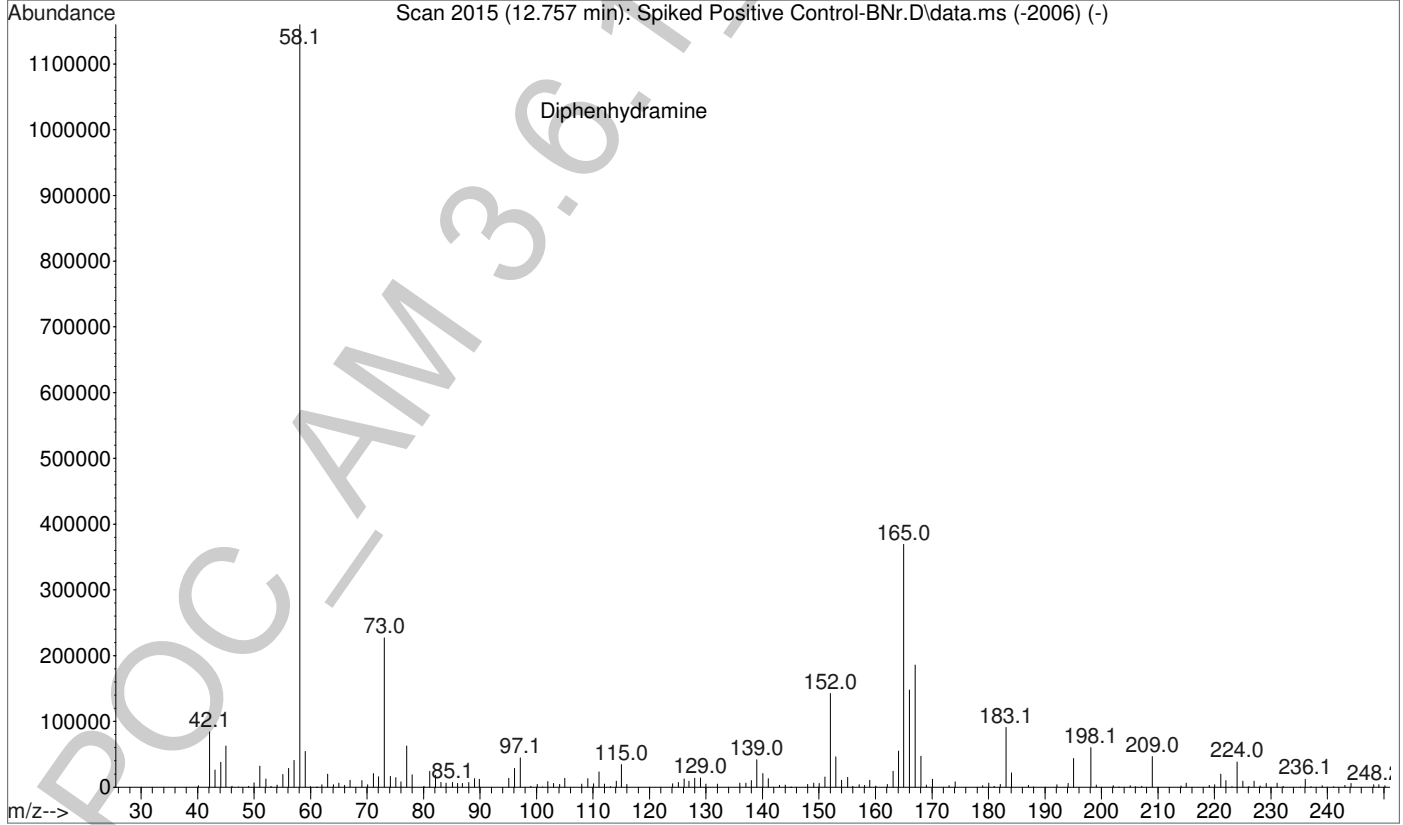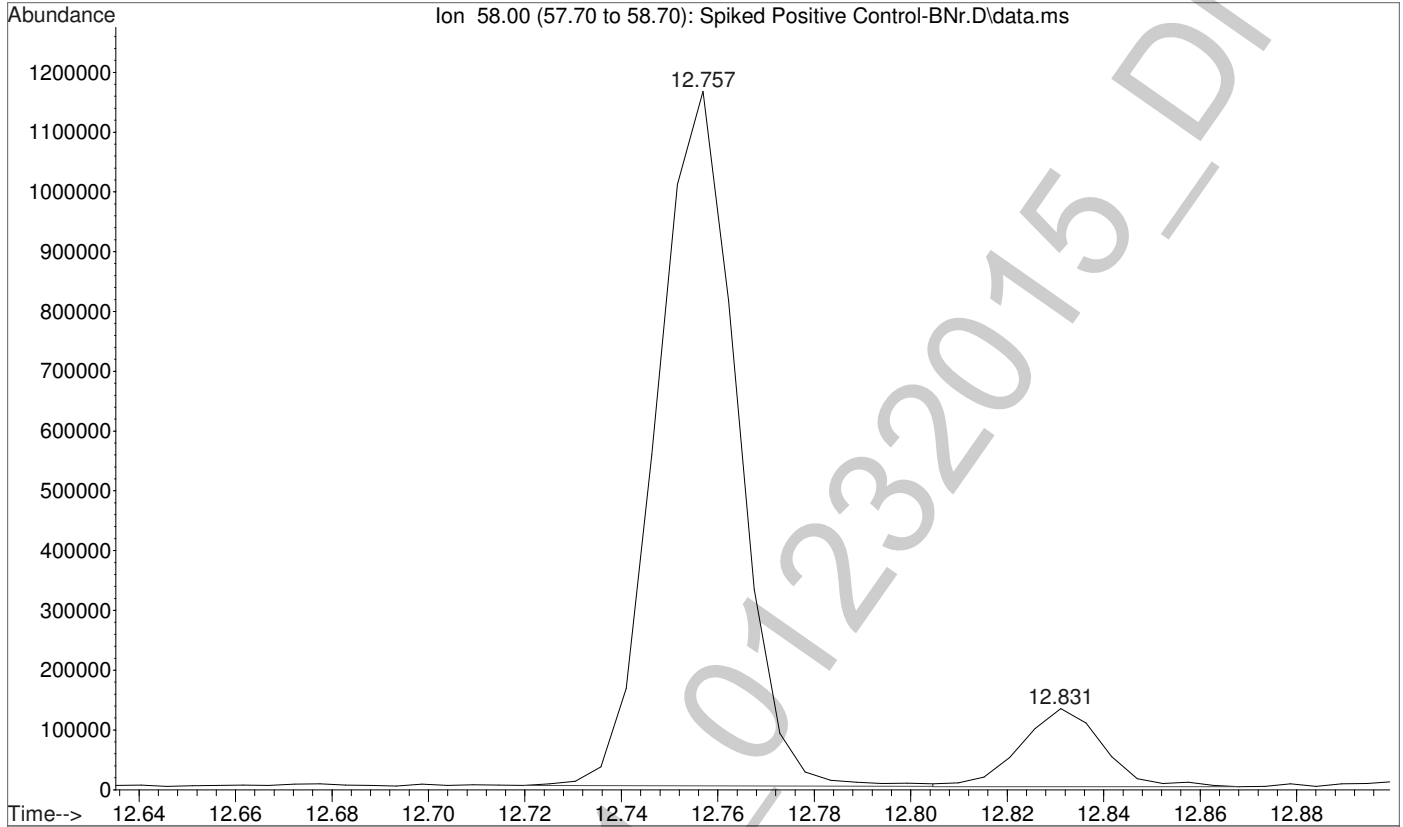



File :C:\gcms\1\data\Blood\012315BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 23 Jan 2015 19:29 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

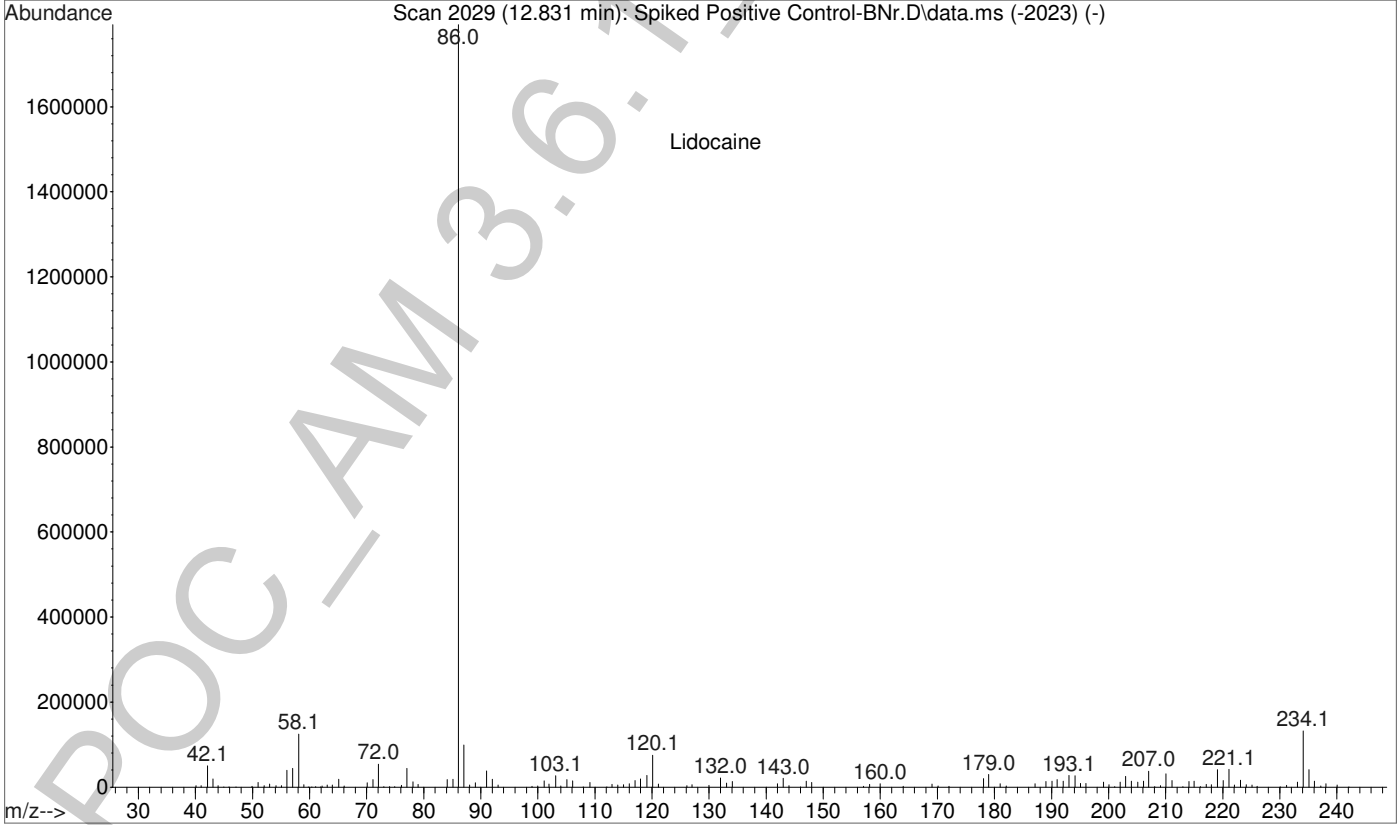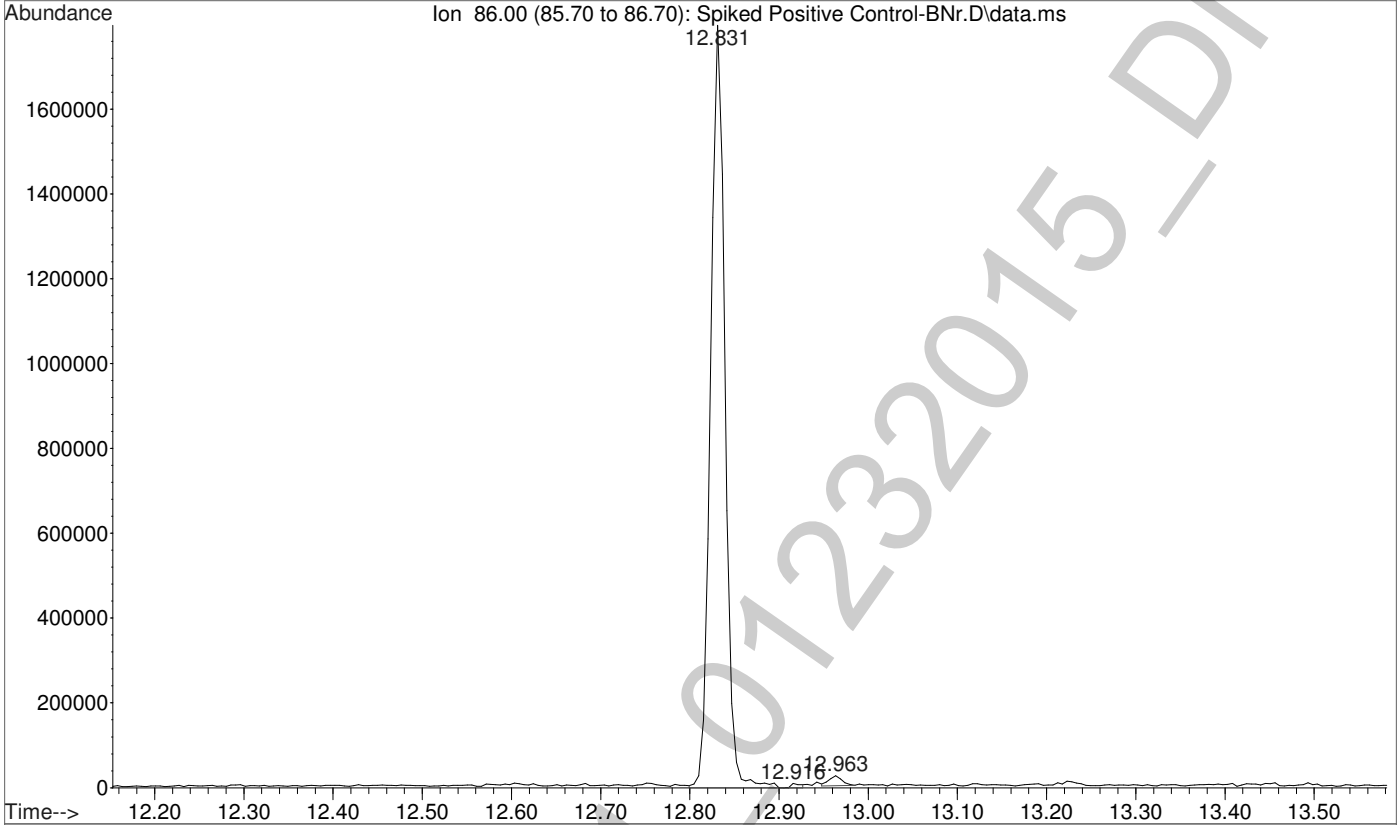



File :C:\gcms\1\data\Blood\012315BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 23 Jan 2015 19:29 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

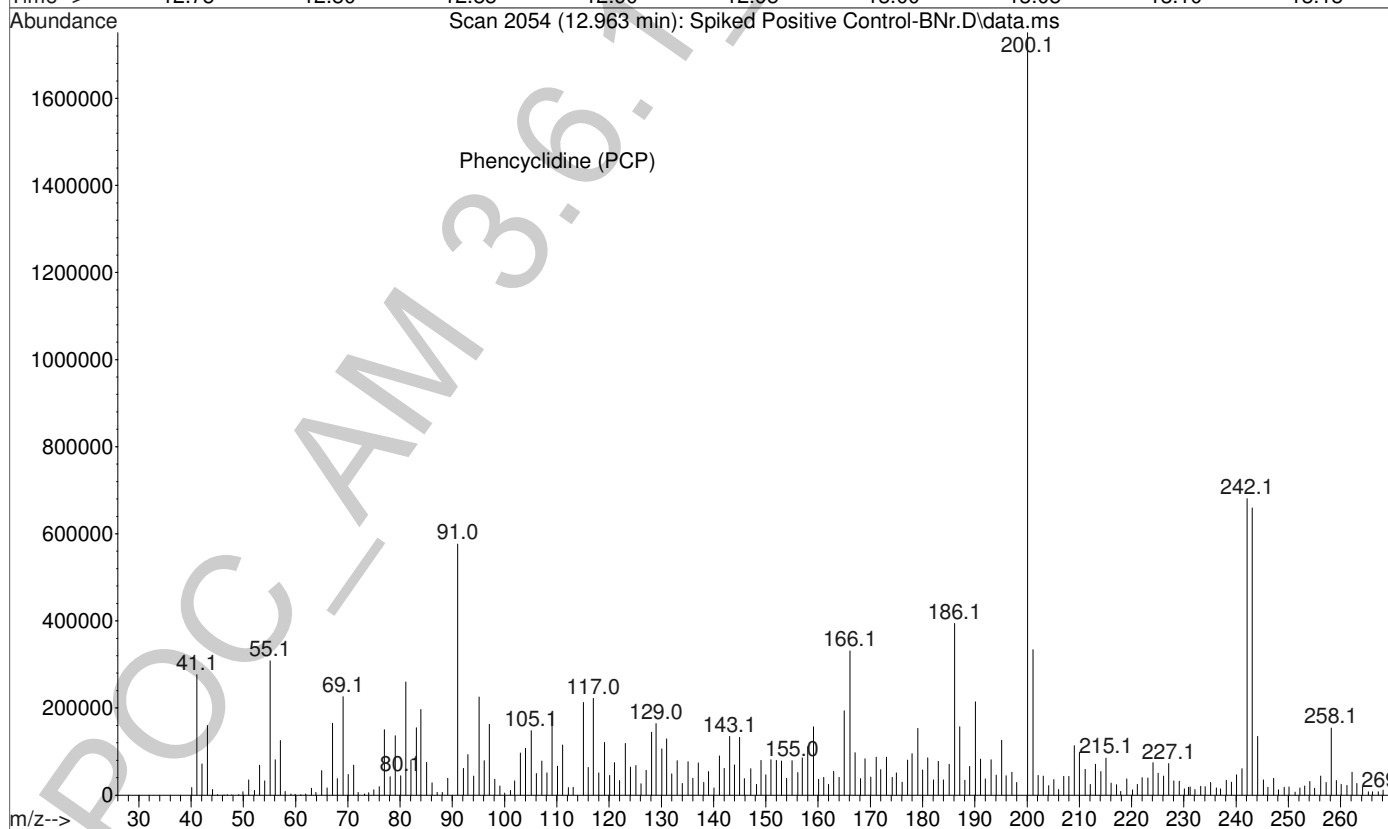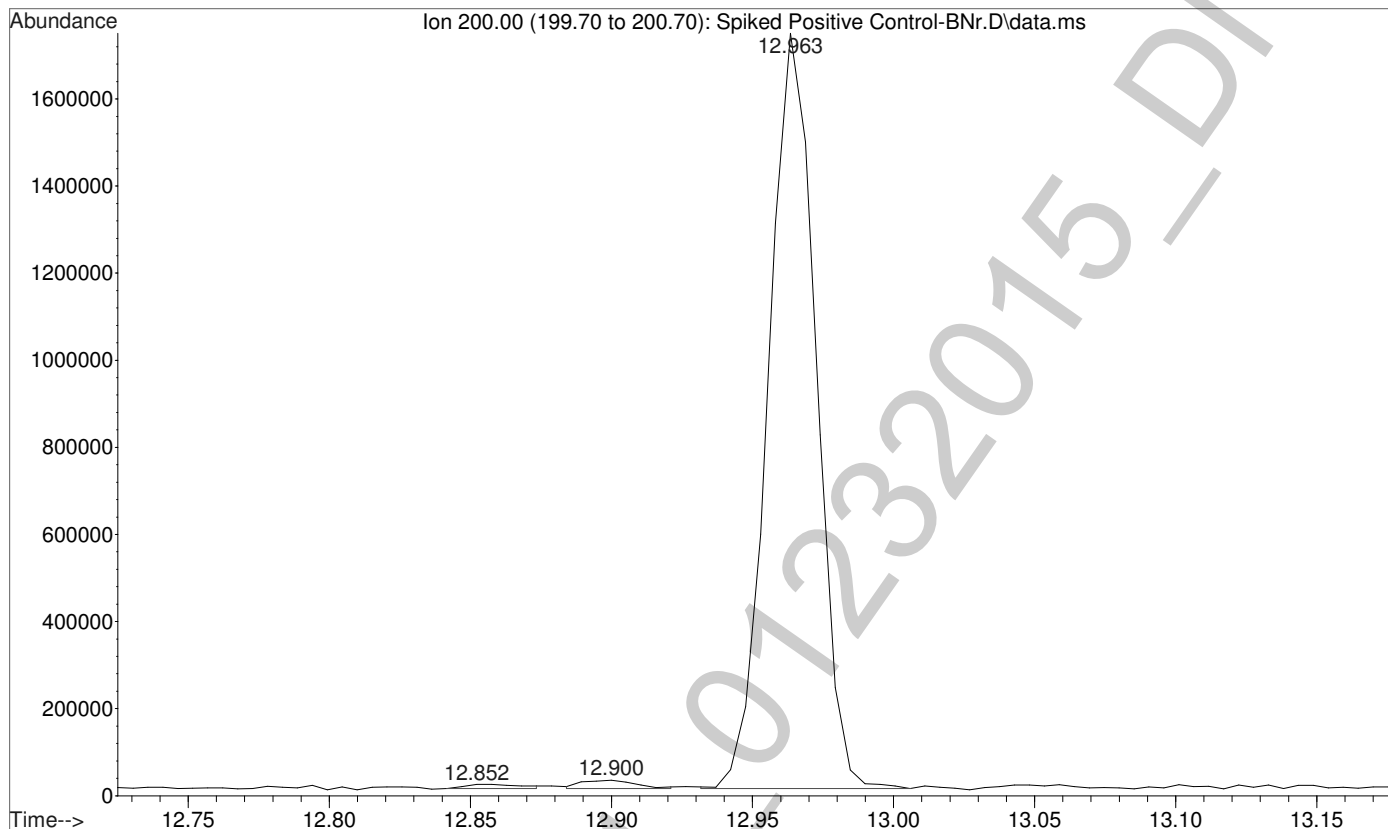



File :C:\gcms\1\data\Blood\012315BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 23 Jan 2015 19:29 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

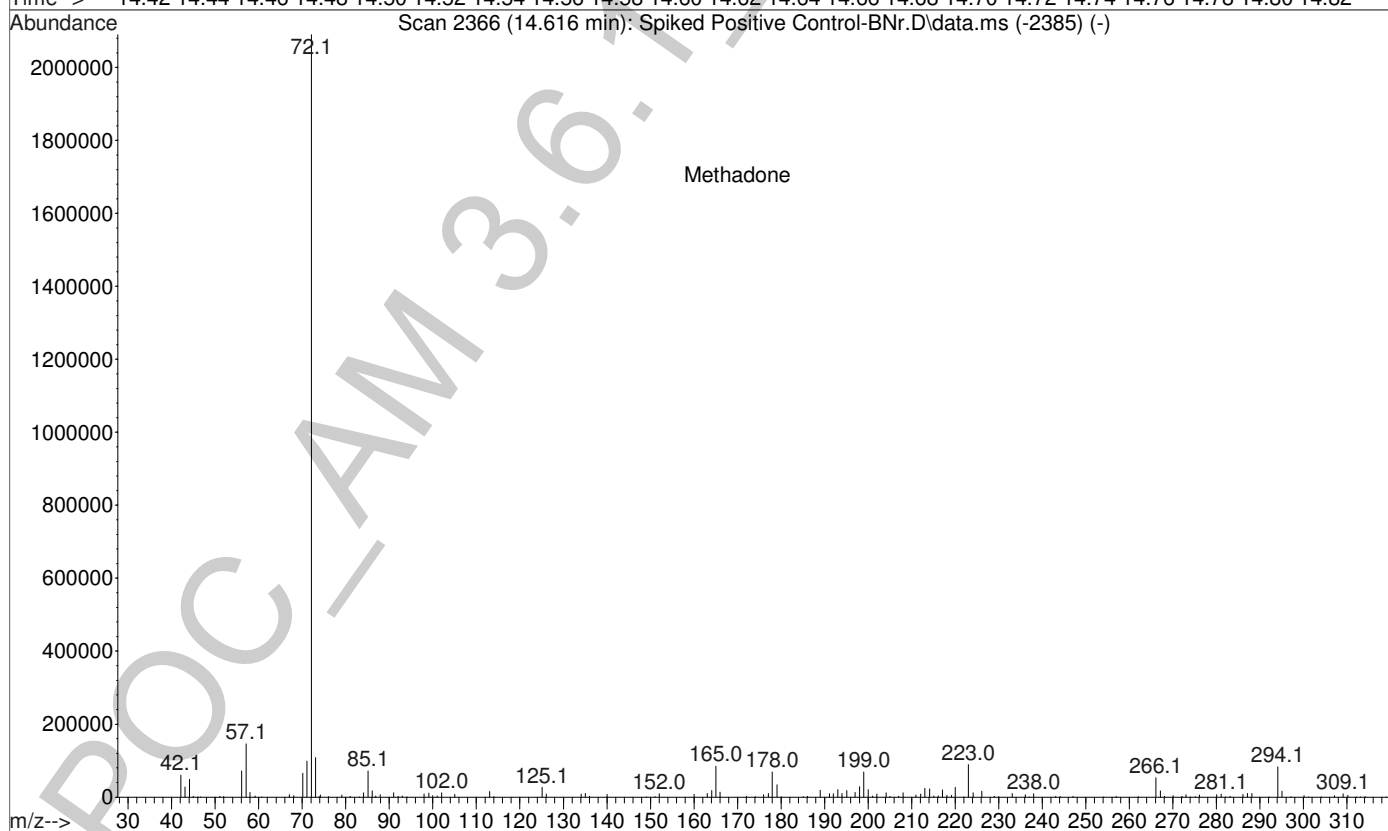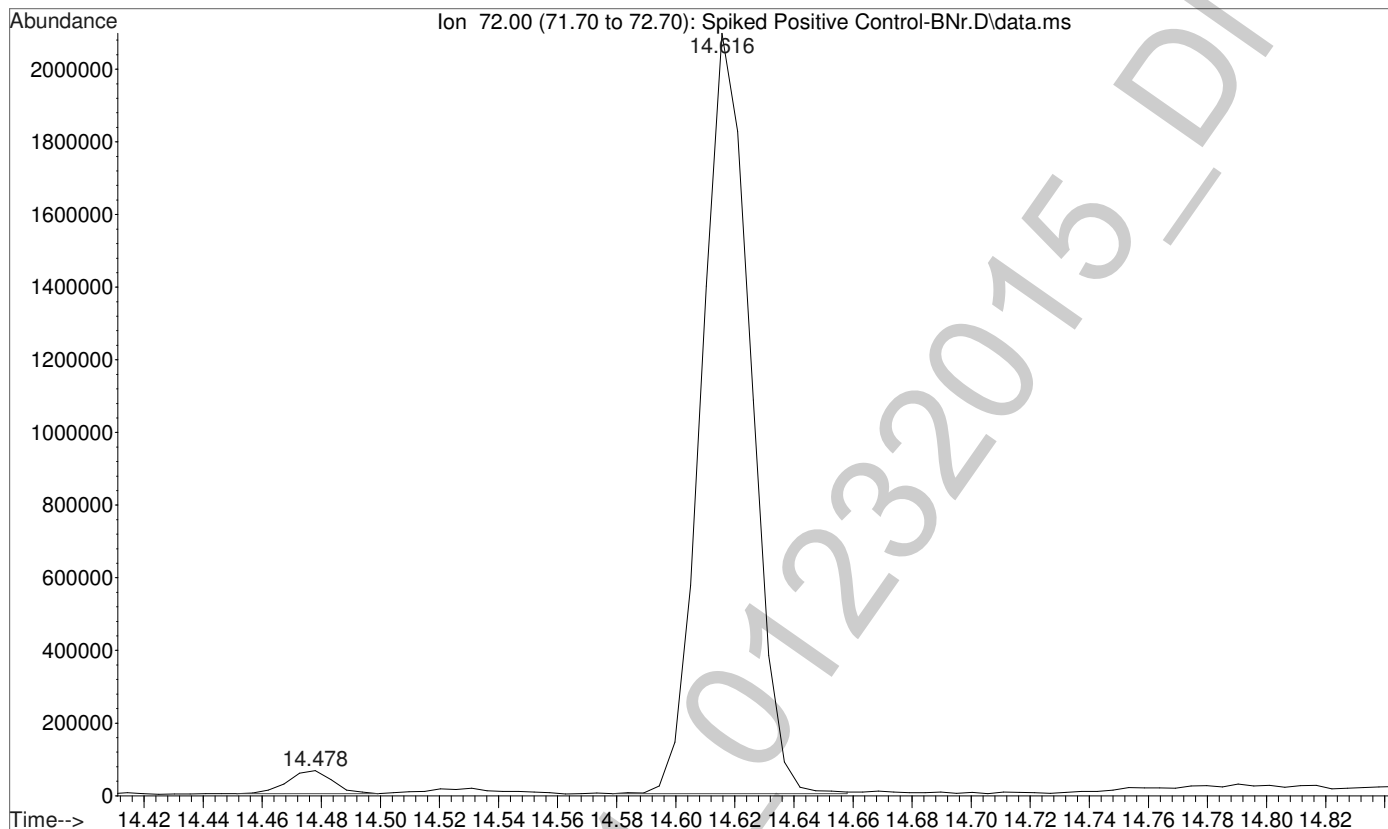



File :C:\gcms\1\data\Blood\012315BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 23 Jan 2015 19:29 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

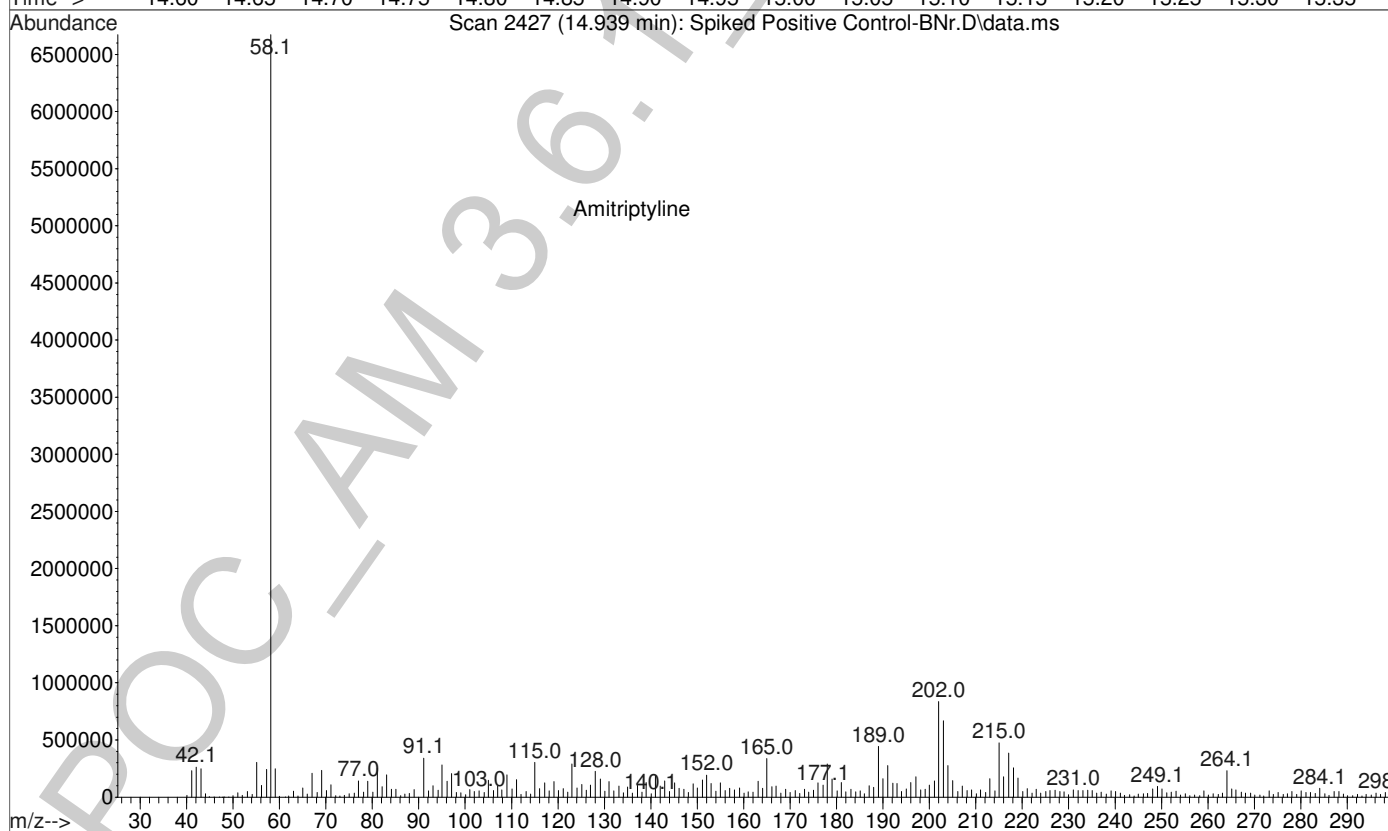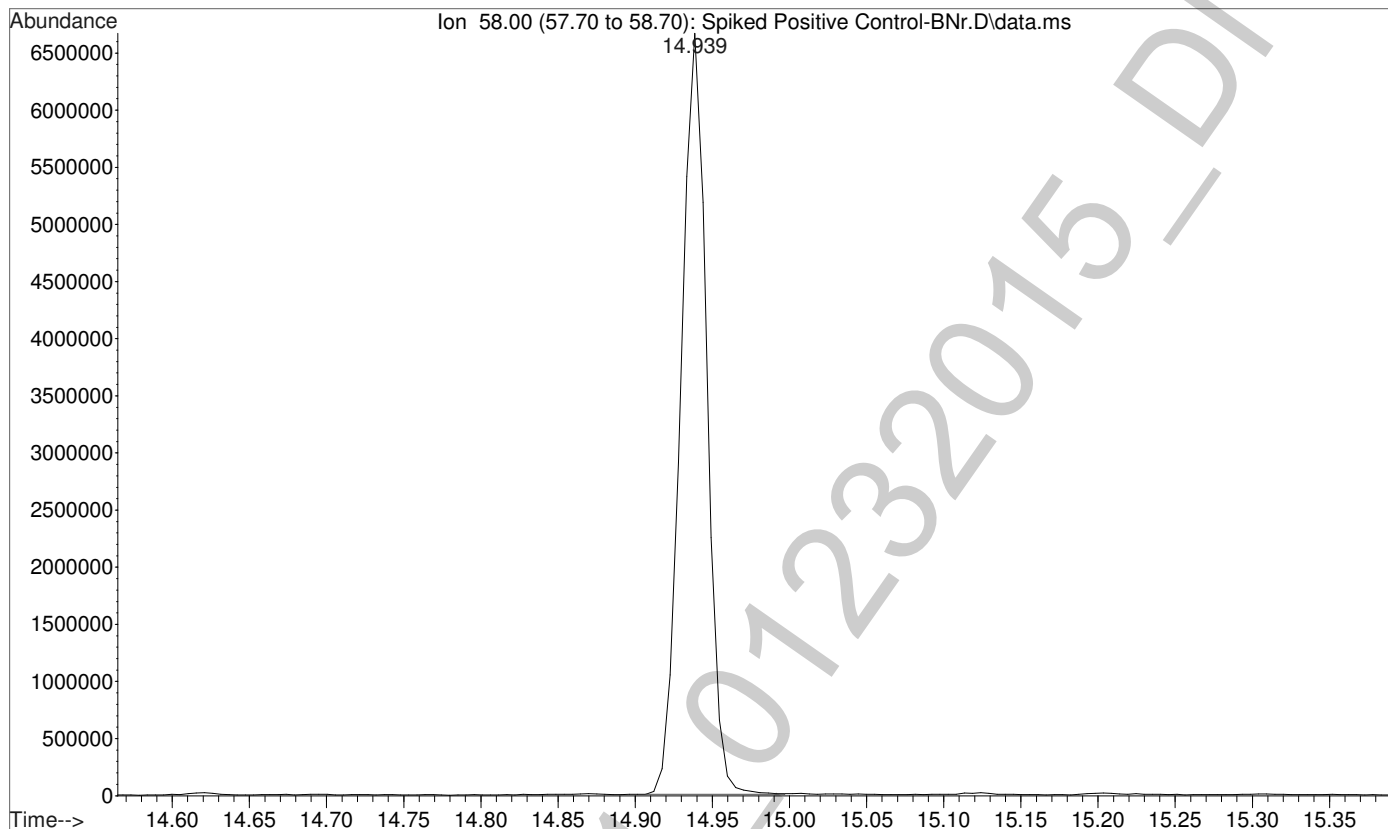



File :C:\gcms\1\data\Blood\012315BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 23 Jan 2015 19:29 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

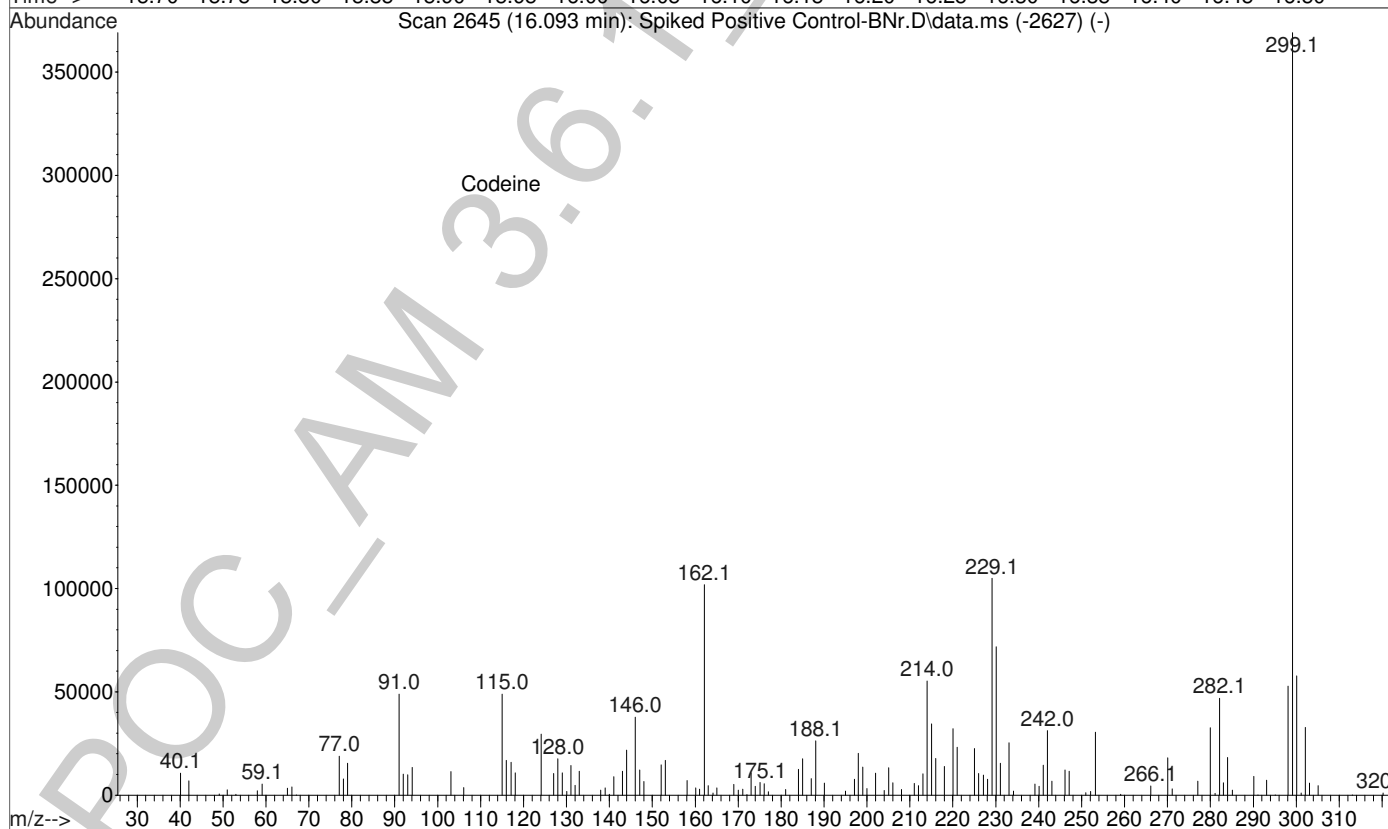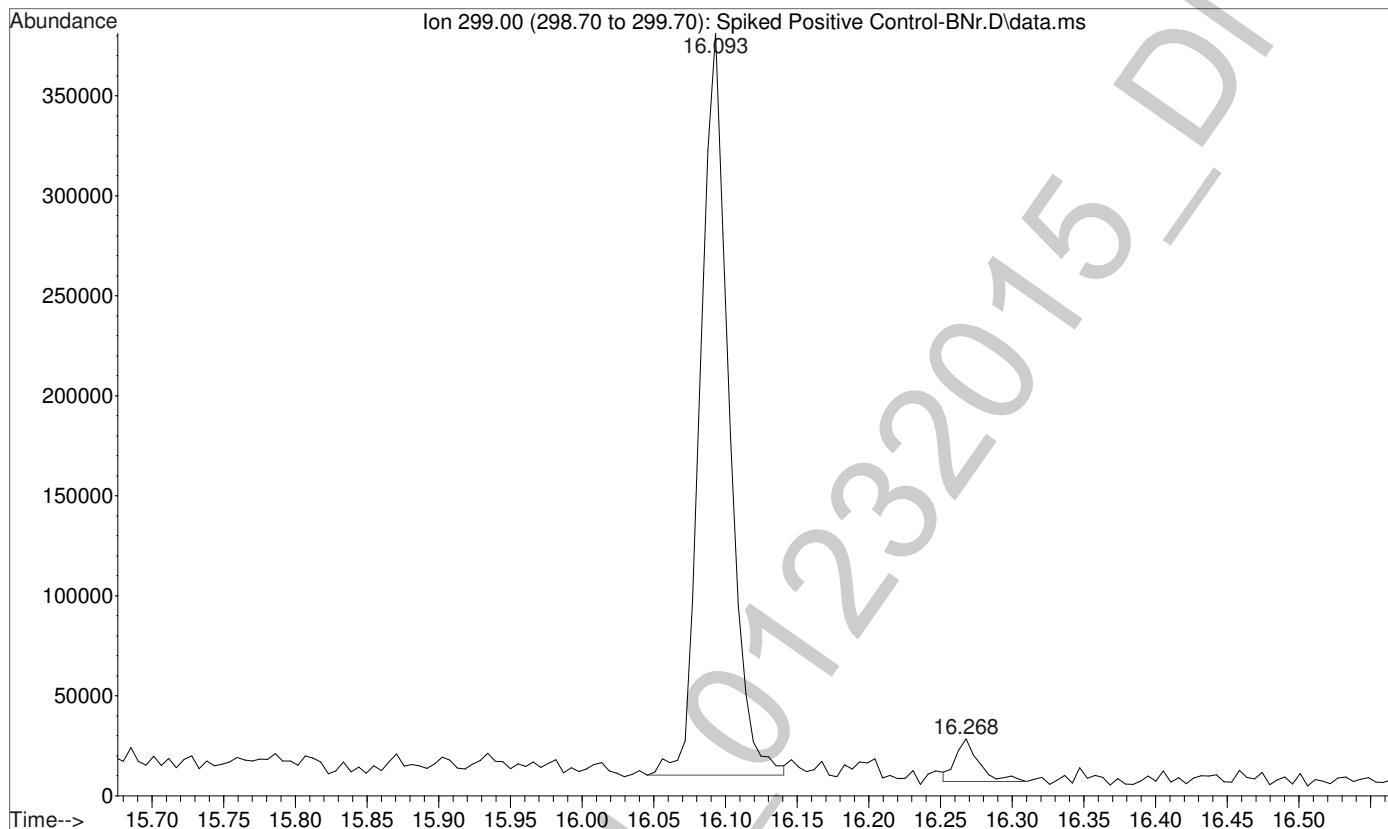



File :C:\gcms\1\data\Blood\012315BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 23 Jan 2015 19:29 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

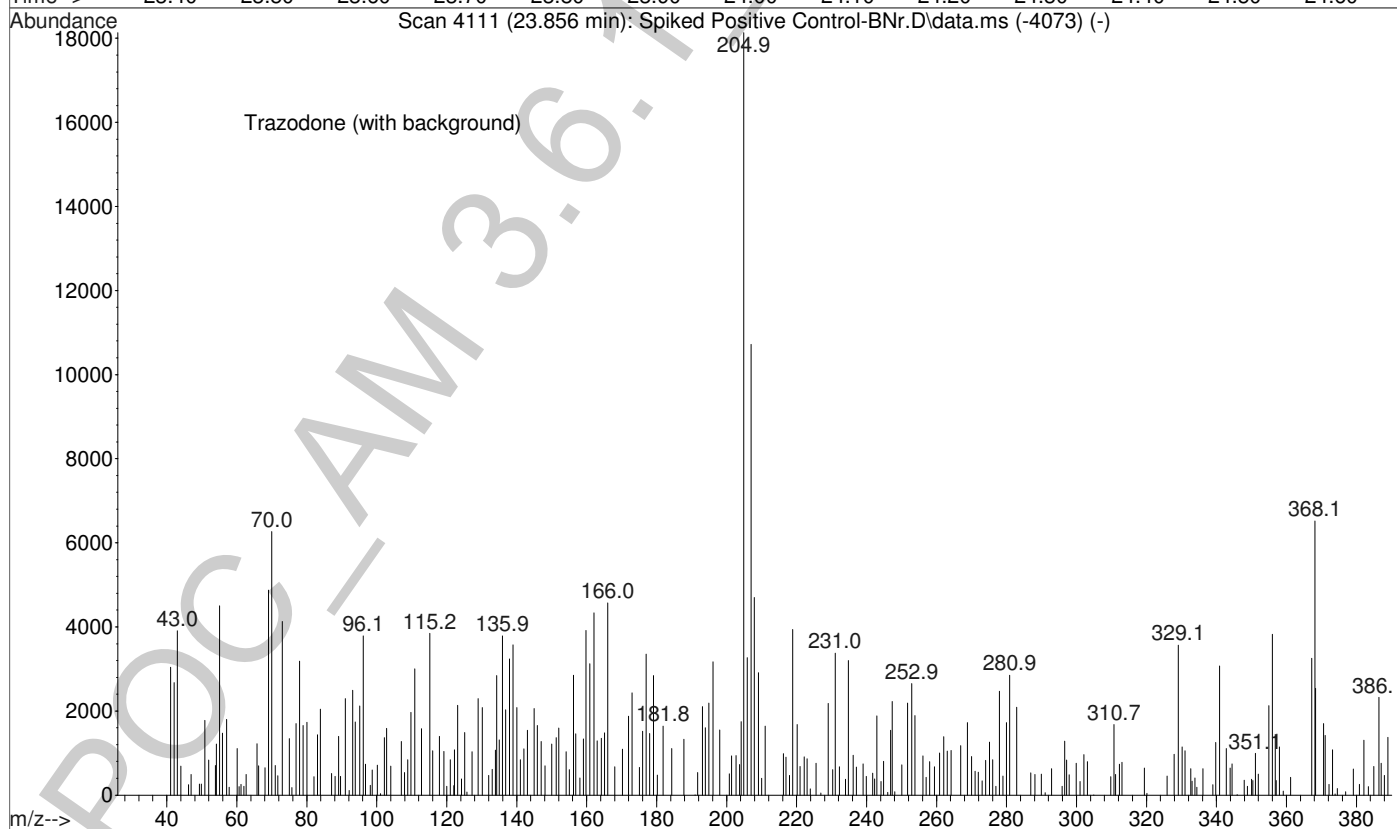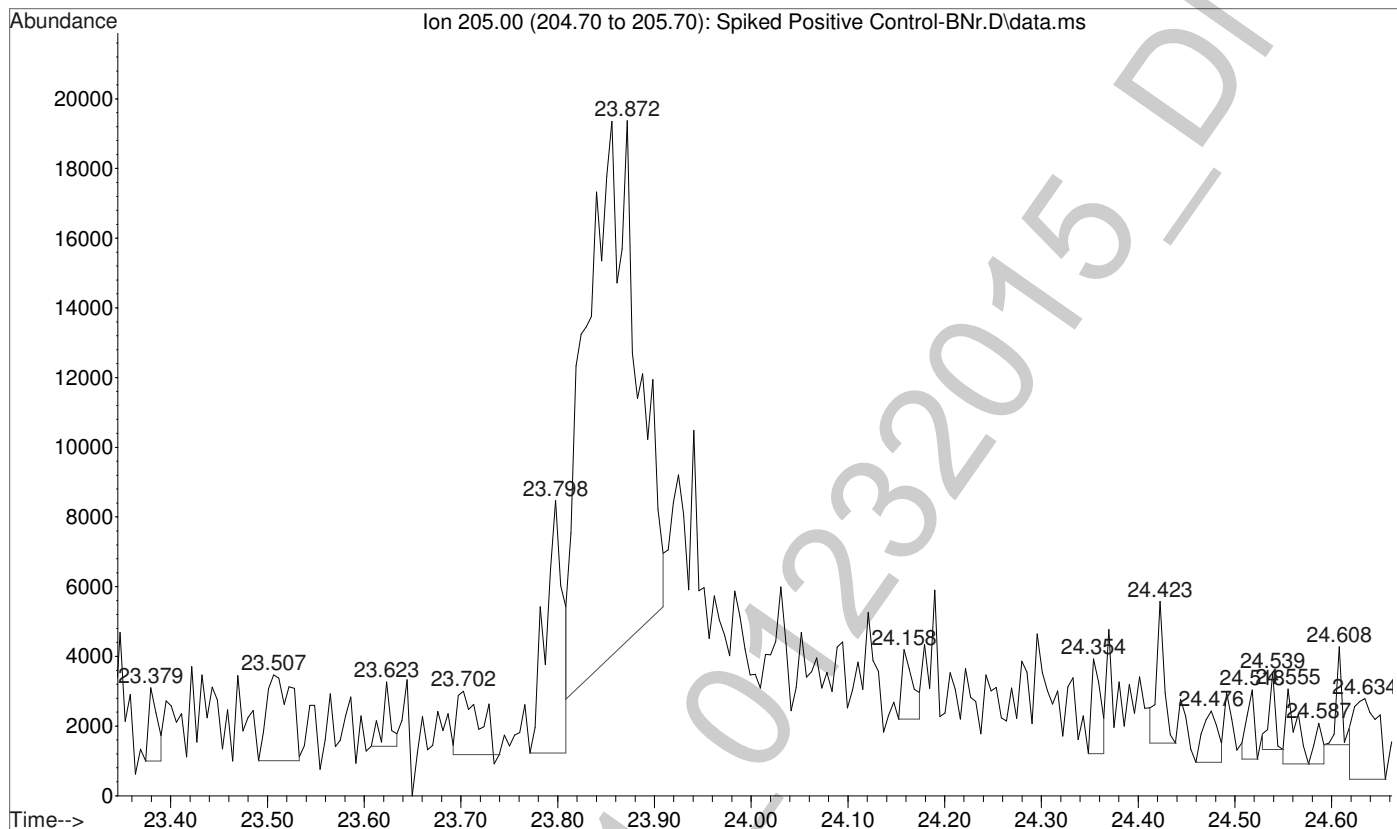



File :C:\gcms\1\data\Blood\012315BN\Reinjection Longer GC Method\p
... rbLK2r.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 23 Jan 2015 20:03 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Solvent Blank
Misc Info : Chloroform

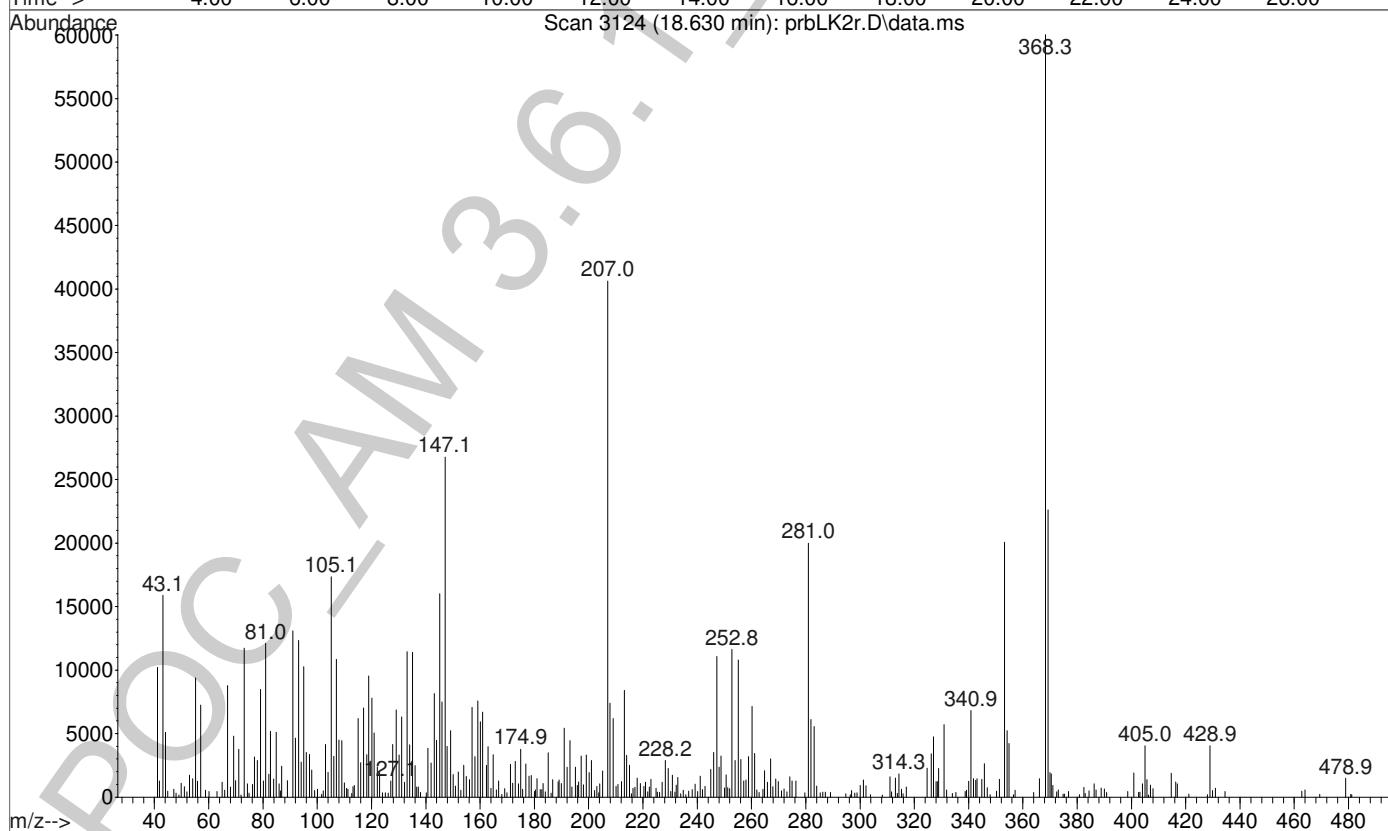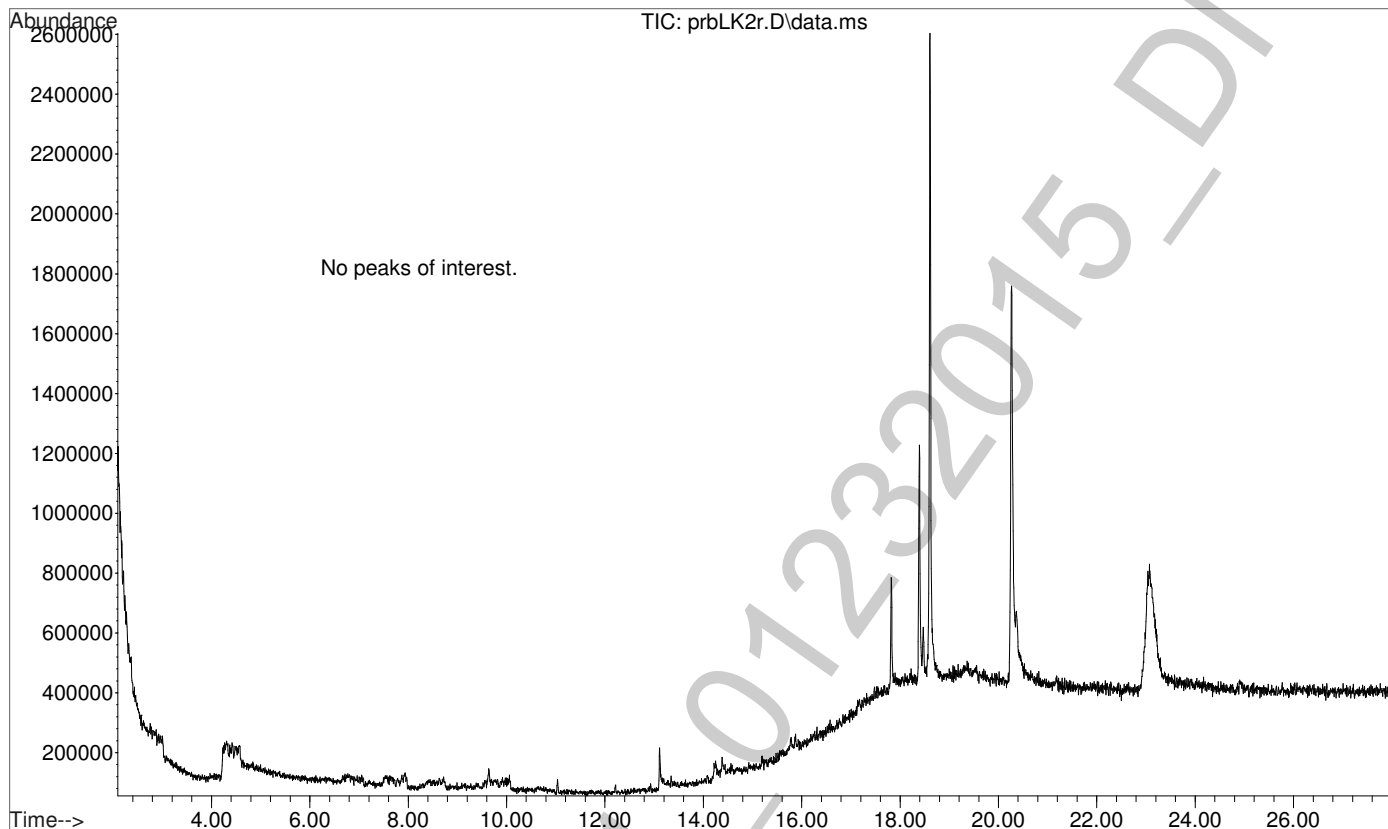

File :C:\gcms\1\data\Blood\012315BN\POSTBLK.D
Operator : 5LAB-C01\ISPuser
Acquired : 25 Jan 2015 18:15 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: BLK
Misc Info : Chloroform
Vial Number: 73

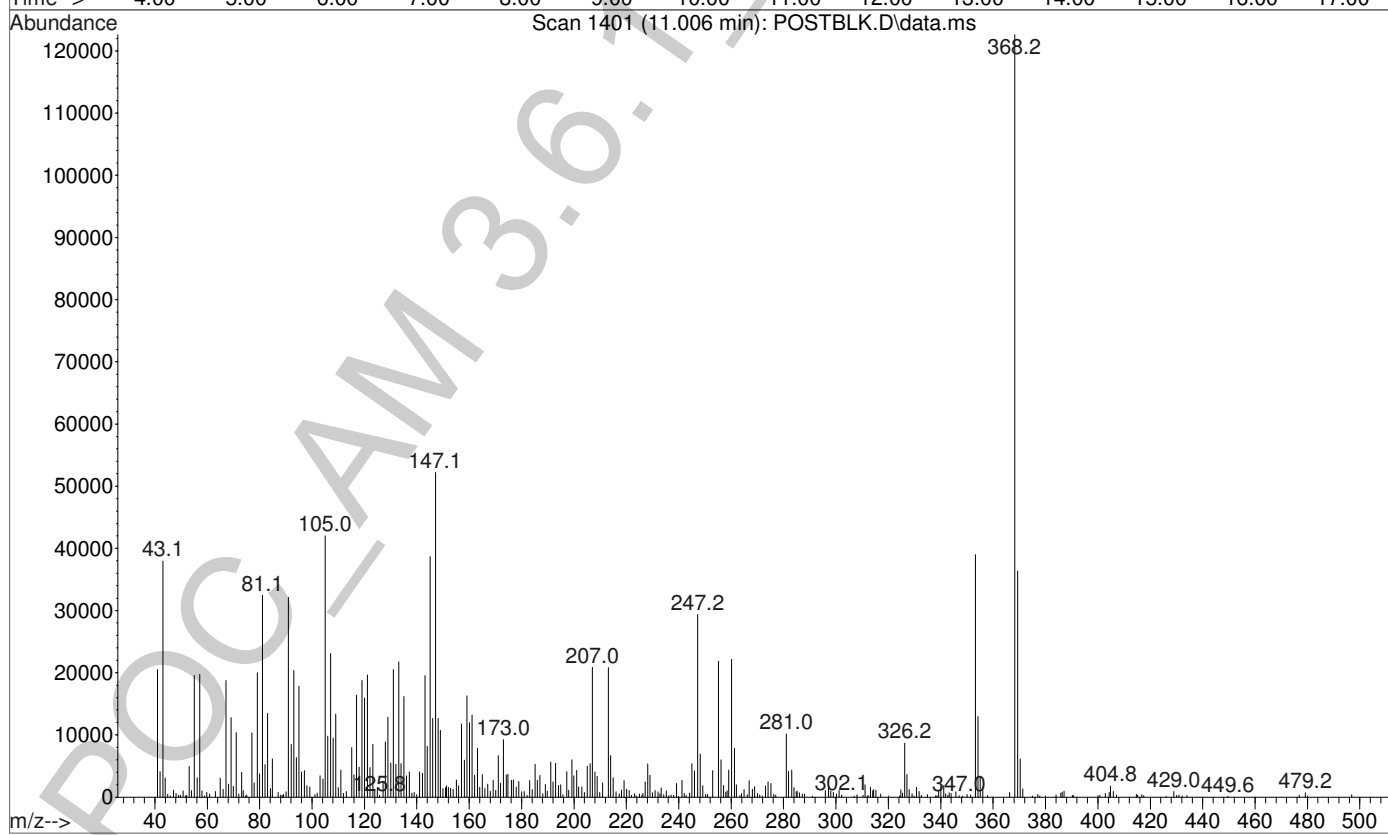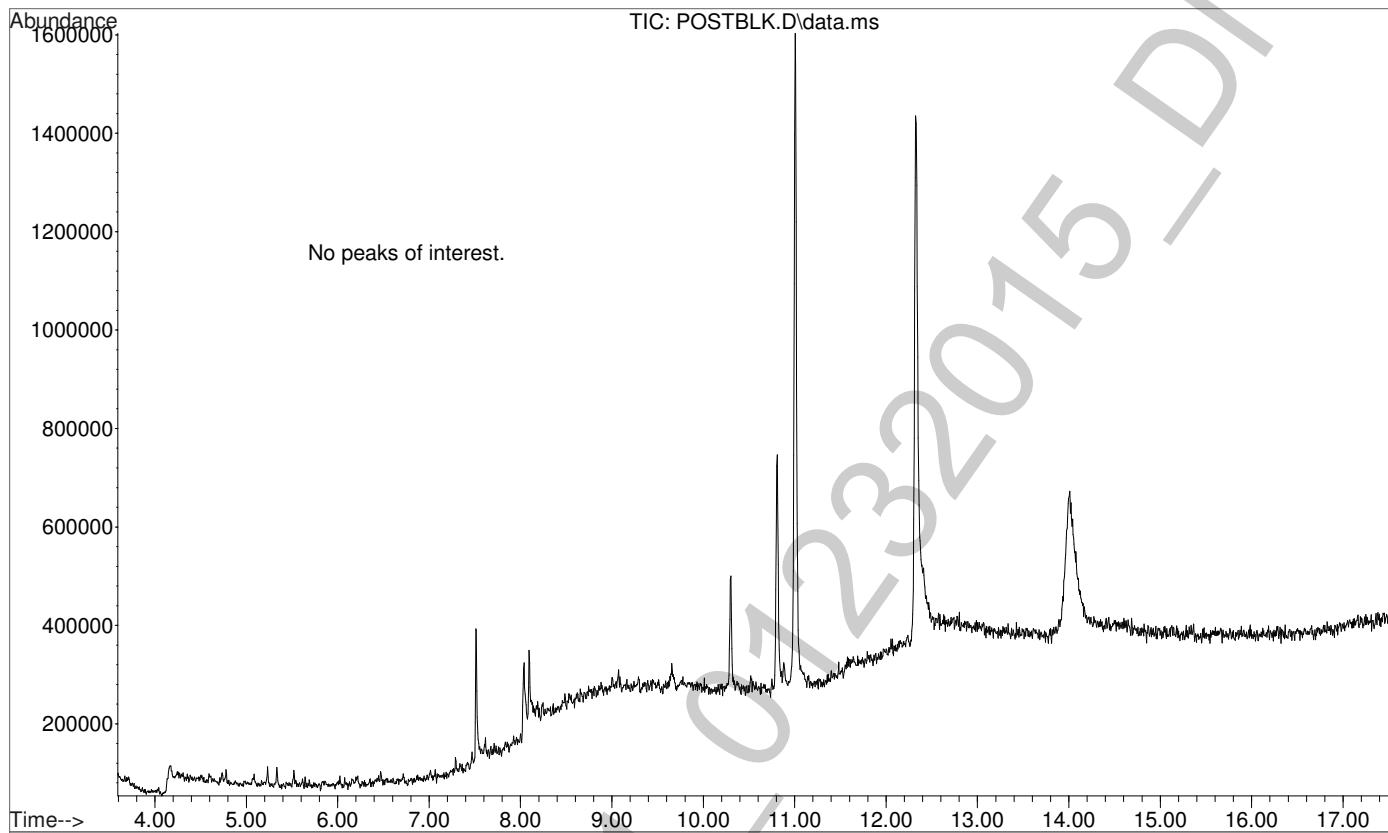

File :C:\gcms\1\data\Blood\012315BN\Reinjection Longer GC Method\P
... rerun Solvent Blankr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 23 Jan 2015 18:21 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Pre-run Solvent Blank
Misc Info : Chloroform

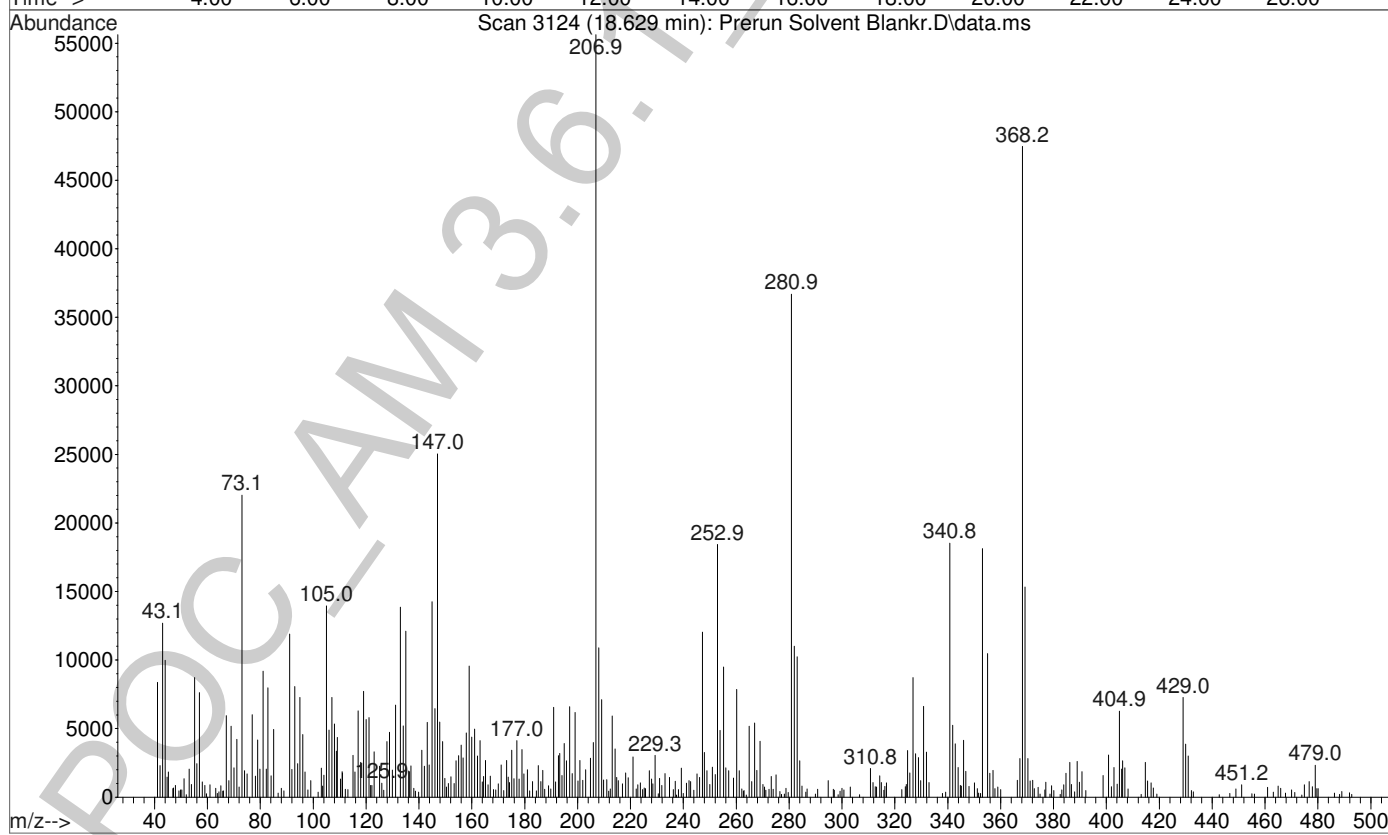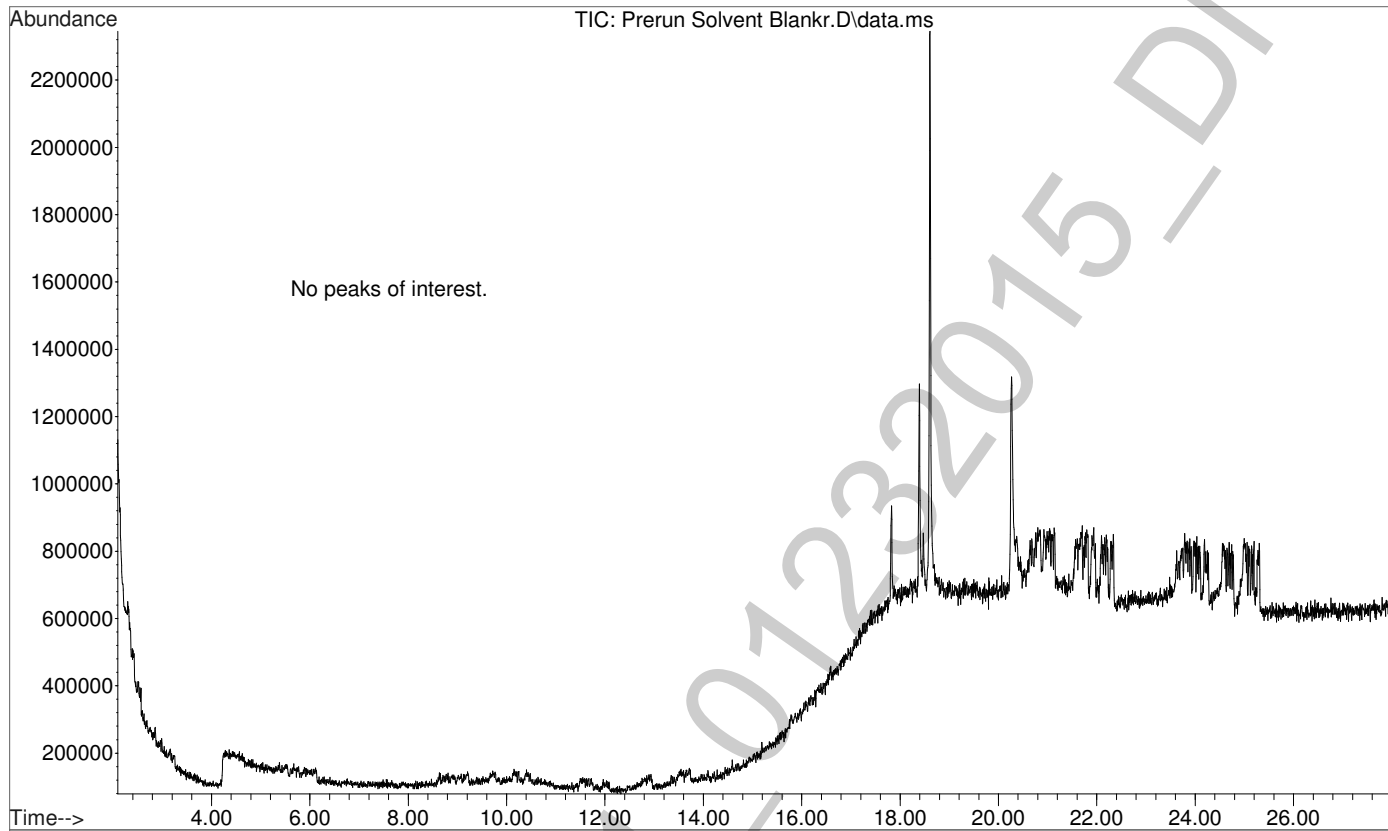

File :C:\gcms\1\data\Blood\012315BN\AFTER.D
Operator : 5LAB-C01\ISPuser
Acquired : 25 Jan 2015 18:37 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: BLK
Misc Info : Chloroform
Vial Number: 72

