

**Worklist: 651**

Also reviewed by AMN (date noted in case files she reviewed). 07/09/2015

<u>LAB_CASE</u>	<u>ITEM</u>	<u>TASK_ID</u>	<u>DESCRIPTION</u>	
M2015-0563	1	28714	3.6.1 Blood base neutral confirr	
M2015-0565	1	28718	3.6.1 Blood base neutral confirr	
M2015-0618	1	29057	3.6.1 Blood base neutral confirr	
M2015-0618	2	29563	3.6.1 Blood base neutral confirr	
M2015-0619	1	29064	3.6.1 Blood base neutral confirr	
M2015-0719	1	29509	3.6.1 Blood base neutral confirr	
M2015-0772	1	29761	3.6.1 Blood base neutral confirr	
M2015-0851	2	30094	3.6.1 Blood base neutral confirr	
P2015-0603	2	31200	3.6.1 Blood base neutral confirr	
P2015-0727	1	30153	3.6.1 Blood base neutral confirr	
P2015-0728	1	30159	3.6.1 Blood base neutral confirr	
P2015-0729	1	30177	3.6.1 Blood base neutral confirr	
P2015-0733	1	30259	3.6.1 Blood base neutral confirr	
P2015-0743	1	30334	3.6.1 Blood base neutral confirr	
P2015-0745	1	30382	3.6.1 Blood base neutral confirr	
P2015-0762	1	30498	3.6.1 Blood base neutral confirr	
P2015-0806	2	31117	3.6.1 Blood base neutral confirr	
P2015-0811	2	30943	3.6.1 Blood base neutral confirr	
P2015-0812	1	30953	3.6.1 Blood base neutral confirr	
P2015-0813	1	30956	3.6.1 Blood base neutral confirr	
P2015-0818	1	30970	3.6.1 Blood base neutral confirr	
P2015-0819	1	30975	3.6.1 Blood base neutral confirr	
P2015-0826	1	31044	3.6.1 Blood base neutral confirr	



**Worklist: 651**

<u>LAB CASE</u>	<u>ITEM</u>	<u>TASK ID</u>	<u>DESCRIPTION</u>
P2015-0832	1	31105	3.6.1 Blood base neutral confir



A handwritten signature in black ink, appearing to be a stylized 'R' or similar character.

POC\_AM 3.6.1\_04012015\_DML

04/01/15  
re

simulate\_sequence.log  
Simulate Run Sequence Wed Apr 01 21:15:45 2015

Instrument Name: Major Mass Spec  
Sequence File: C:\Users\ISPuser\Desktop\Sequences\DD-BNSB.sequence.xml  
Comment: MassHunter sequence  
Operator: 5LAB-C01\ISPuser  
Data Path: D:\DATA\DND\2015\040115BN\  
Method Path: D:\MassHunter\GCMS\1\methods\

Line	Type	Vials	DataFile	Sample Name
Acquisition Method: BNSB120510.M				
1)	Sample	100	Prerun Solvent Blank	Pre-run Solvent Blank
2)	Sample	1	Negative Control-BN	Negative Control -
...0130				
3)	Sample	2	Spiked Positive Control-BN	Positive Control
4)	Sample	99	prbLK2	Solvent Blank
Acquisition Method: GBT092509-Delta EMV.M				
5)	Sample	100	Prerun Solvent Blankr	Pre-run Solvent Blank
6)	Sample	1	Negative Control-BNr	Negative Control -
...0130				
7)	Sample	2	Spiked Positive Control-BNr	Positive Control
8)	Sample	99	prbLK2r	Solvent Blank
Acquisition Method: BNSB120510.M				
9)	Sample	98	P2015-0695-2-BNBLK	Lab No.:
P2015-069...tion				
10)	Sample	3	P2015-0695-2-BN	Lab No.:
P2015-069...tion				
11)	Sample	97	P2015-0695-3-BNBLK	Lab No.:
P2015-069...tion				
12)	Sample	4	P2015-0695-3-BN	Lab No.:
P2015-069...tion				
13)	Sample	96	M2015-0563-1-BNBLK	Lab No.: M2015-0563-1
14)	Sample	5	M2015-0563-1-BN	Lab No.: M2015-0563-1
15)	Sample	95	M2015-0565-1-BNBLK	Lab No.: M2015-0565-1
16)	Sample	6	M2015-0565-1-BN	Lab No.: M2015-0565-1
17)	Sample	94	M2015-0618-1-BNBLK	Lab No.: M2015-0618-1
18)	Sample	7	M2015-0618-1-BN	Lab No.: M2015-0618-1
19)	Sample	93	M2015-0618-2-BNBLK	Lab No.: M2015-0618-2
20)	Sample	8	M2015-0618-2-BN	Lab No.: M2015-0618-2
21)	Sample	92	M2015-0619-1-BNBLK	Lab No.: M2015-0619-1
22)	Sample	9	M2015-0619-1-BN	Lab No.: M2015-0619-1
23)	Sample	91	M2015-0719-1-BNBLK	Lab No.: M2015-0719-1
24)	Sample	10	M2015-0719-1-BN	Lab No.: M2015-0719-1
Acquisition Method: GBT092509-Delta EMV.M				
25)	Sample	98	P2015-0695-2-BNBLKr	Lab No.:
P2015-069...tion				
26)	Sample	3	P2015-0695-2-BNr	Lab No.:
P2015-069...tion				
27)	Sample	97	P2015-0695-3-BNBLKr	Lab No.:
P2015-069...tion				
28)	Sample	4	P2015-0695-3-BNr	Lab No.:
P2015-069...tion				
29)	Sample	96	M2015-0563-1-BNBLKr	Lab No.: M2015-0563-1
30)	Sample	5	M2015-0563-1-BNr	Lab No.: M2015-0563-1
31)	Sample	95	M2015-0565-1-BNBLKr	Lab No.: M2015-0565-1
32)	Sample	6	M2015-0565-1-BNr	Lab No.: M2015-0565-1
33)	Sample	94	M2015-0618-1-BNBLKr	Lab No.: M2015-0618-1
34)	Sample	7	M2015-0618-1-BNr	Lab No.: M2015-0618-1
35)	Sample	93	M2015-0618-2-BNBLKr	Lab No.: M2015-0618-2
36)	Sample	8	M2015-0618-2-BNr	Lab No.: M2015-0618-2
37)	Sample	92	M2015-0619-1-BNBLKr	Lab No.: M2015-0619-1
38)	Sample	9	M2015-0619-1-BNr	Lab No.: M2015-0619-1

Insufficient sample - removed from sequence. &

04/01/15

simulate\_sequence.log

39) Sample	✓91	M2015-0719-1-BNBLKr	Lab No.:	M2015-0719-1
40) Sample	✓10	M2015-0719-1-BNr	Lab No.:	M2015-0719-1

Acquisition Method: BNSB120510.M

41) Sample	✓90	M2015-0772-1-BNBLK	Lab No.:	M2015-0772-1
42) Sample	✓11	M2015-0772-1-BN	Lab No.:	M2015-0772-1
43) Sample	✓89	M2015-0851-2-BNBLK	Lab No.:	M2015-0851-2
44) Sample	✓12	M2015-0851-2-BN	Lab No.:	M2015-0851-2
45) Sample	✓88	P2015-0603-2-BNBLK	Lab No.:	P2015-0603-2
46) Sample	✓13	P2015-0603-2-BN	Lab No.:	P2015-0603-2
47) Sample	✓87	P2015-0727-1-BNBLK	Lab No.:	P2015-0727-1
48) Sample	✓14	P2015-0727-1-BN	Lab No.:	P2015-0727-1
49) Sample	✓86	P2015-0728-1-BNBLK	Lab No.:	P2015-0728-1
50) Sample	✓15	P2015-0728-1-BN	Lab No.:	P2015-0728-1

Acquisition Method: GBT092509-Delta EMV.M

51) Sample	✓90	M2015-0772-1-BNBLKr	Lab No.:	M2015-0772-1
52) Sample	✓11	M2015-0772-1-BNr	Lab No.:	M2015-0772-1
53) Sample	✓89	M2015-0851-2-BNBLKr	Lab No.:	M2015-0851-2
54) Sample	✓12	M2015-0851-2-BNr	Lab No.:	M2015-0851-2
55) Sample	✓88	P2015-0603-2-BNBLKr	Lab No.:	P2015-0603-2
56) Sample	✓13	P2015-0603-2-BNr	Lab No.:	P2015-0603-2
57) Sample	✓87	P2015-0727-1-BNBLKr	Lab No.:	P2015-0727-1
58) Sample	✓14	P2015-0727-1-BNr	Lab No.:	P2015-0727-1
59) Sample	✓86	P2015-0728-1-BNBLKr	Lab No.:	P2015-0728-1
60) Sample	✓15	P2015-0728-1-BNr	Lab No.:	P2015-0728-1

Acquisition Method: BNSB120510.M

61) Sample	✓85	P2015-0729-1-BNBLK	Lab No.:	P2015-0729-1
62) Sample	✓16	P2015-0729-1-BN	Lab No.:	P2015-0729-1
63) Sample	✓84	P2015-0733-1-BNBLK	Lab No.:	P2015-0733-1
64) Sample	✓17	P2015-0733-1-BN	Lab No.:	P2015-0733-1
65) Sample	✓83	P2015-0743-1-BNBLK	Lab No.:	P2015-0743-1
66) Sample	✓18	P2015-0743-1-BN	Lab No.:	P2015-0743-1
* 67) Sample	✓82	P2015-0744-1-BNBLK	Lab No.:	P2015-0744-1
* 68) Sample	✓19	P2015-0744-1-BN	Lab No.:	P2015-0744-1
69) Sample	✓81	P2015-0745-1-BNBLK	Lab No.:	P2015-0745-1
70) Sample	✓20	P2015-0745-1-BN	Lab No.:	P2015-0745-1

Acquisition Method: GBT092509-Delta EMV.M

71) Sample	✓85	P2015-0729-1-BNBLKr	Lab No.:	P2015-0729-1
72) Sample	✓16	P2015-0729-1-BNr	Lab No.:	P2015-0729-1
73) Sample	✓84	P2015-0733-1-BNBLKr	Lab No.:	P2015-0733-1
74) Sample	✓17	P2015-0733-1-BNr	Lab No.:	P2015-0733-1
75) Sample	✓83	P2015-0743-1-BNBLKr	Lab No.:	P2015-0743-1
76) Sample	✓18	P2015-0743-1-BNr	Lab No.:	P2015-0743-1
* 77) Sample	✓82	P2015-0744-1-BNBLKr	Lab No.:	P2015-0744-1
* 78) Sample	✓19	P2015-0744-1-BNr	Lab No.:	P2015-0744-1
79) Sample	✓81	P2015-0745-1-BNBLKr	Lab No.:	P2015-0745-1
80) Sample	✓20	P2015-0745-1-BNr	Lab No.:	P2015-0745-1

Acquisition Method: BNSB120510.M

81) Sample	✓80	P2015-0762-1-BNBLK	Lab No.:	P2015-0762-1
82) Sample	✓21	P2015-0762-1-BN	Lab No.:	P2015-0762-1
83) Sample	✓79	P2015-0806-2-BNBLK	Lab No.:	P2015-0806-2
84) Sample	✓22	P2015-0806-2-BN	Lab No.:	P2015-0806-2
85) Sample	✓78	P2015-0811-2-BNBLK	Lab No.:	P2015-0811-2
86) Sample	✓23	P2015-0811-2-BN	Lab No.:	P2015-0811-2
87) Sample	✓77	P2015-0812-1-BNBLK	Lab No.:	P2015-0812-1
88) Sample	✓24	P2015-0812-1-BN	Lab No.:	P2015-0812-1
89) Sample	✓76	P2015-0813-1-BNBLK	Lab No.:	P2015-0813-1
90) Sample	✓25	P2015-0813-1-BN	Lab No.:	P2015-0813-1

Acquisition Method: GBT092509-Delta EMV.M

91) Sample	✓80	P2015-0762-1-BNBLKr	Lab No.:	P2015-0762-1
92) Sample	✓21	P2015-0762-1-BNr	Lab No.:	P2015-0762-1
93) Sample	✓79	P2015-0806-2-BNBLKr	Lab No.:	P2015-0806-2
94) Sample	✓22	P2015-0806-2-BNr	Lab No.:	P2015-0806-2

CR 04/01/15

```

simulate_sequence.log
95) Sample /78 P2015-0811-2-BNBLKr Lab No.: P2015-0811-2
96) Sample /23 P2015-0811-2-BNr Lab No.: P2015-0811-2
97) Sample /77 P2015-0812-1-BNBLKr Lab No.: P2015-0812-1
98) Sample /24 P2015-0812-1-BNr Lab No.: P2015-0812-1
99) Sample /76 P2015-0813-1-BNBLKr Lab No.: P2015-0813-1
100) Sample /25 P2015-0813-1-BNr Lab No.: P2015-0813-1

```

```

Acquisition Method: BNSB120510.M
101) Sample /75 P2015-0818-1-BNBLK Lab No.: P2015-0818-1
102) Sample /26 P2015-0818-1-BN Lab No.: P2015-0818-1
103) Sample /74 P2015-0819-1-BNBLK Lab No.: P2015-0819-1
104) Sample /27 P2015-0819-1-BN Lab No.: P2015-0819-1
105) Sample /73 P2015-0826-1-BNBLK Lab No.: P2015-0826-1
106) Sample /28 P2015-0826-1-BN Lab No.: P2015-0826-1
107) Sample /72 P2015-0832-1-BNBLK Lab No.: P2015-0832-1
108) Sample /29 P2015-0832-1-BN Lab No.: P2015-0832-1

```

```

Acquisition Method: GBT092509-Delta EMV.M
109) Sample /75 P2015-0818-1-BNBLKr Lab No.: P2015-0818-1
110) Sample /26 P2015-0818-1-BNr Lab No.: P2015-0818-1
111) Sample /74 P2015-0819-1-BNBLKr Lab No.: P2015-0819-1
112) Sample /27 P2015-0819-1-BNr Lab No.: P2015-0819-1
113) Sample /73 P2015-0826-1-BNBLKr Lab No.: P2015-0826-1
114) Sample /28 P2015-0826-1-BNr Lab No.: P2015-0826-1
115) Sample /72 P2015-0832-1-BNBLKr Lab No.: P2015-0832-1
116) Sample /29 P2015-0832-1-BNr Lab No.: P2015-0832-1

```

```

Acquisition Method: BNSB120510.M
117) Sample /71 POSTBLKr BLK

```

```

Acquisition Method: GBT092509-Delta EMV.M
118) Sample /70 AFTER BLK
megabytes Needed: 2405 Space on drive D: 307550
Sequence Verification Done!

```

POC\_AM 3.6.1-104232

Analytical Method 3.6.1 & 3.6.7 QA Check List

Run Start Date: 04/01/15

Analyst: DND

(Short GC/MS temperature program)

Positive Control Compound List

- Methamphetamine
- Nicotine
- (Meperidine)
- Caffeine
- Diphenhydramine
- Lidocaine
- PCP
- Methadone
- Amitriptyline
- Codeine
- Trazodone



Internal Standards

- Benzphetamine
- Papaverine



Optional back extraction **not** performed.  
Samples reconstituted in methanol.



File :C:\gcms\1\data\Blood\040115BN\Prerun Solvent Blank.D  
Operator : 5LAB-C01\ISPuser  
Acquired : 01 Apr 2015 22:46 using AcqMethod BNSB120510.M  
Instrument : Major Mass Spec  
Sample Name: Pre-run Solvent Blank  
Misc Info : Chloroform  
Vial Number: 100

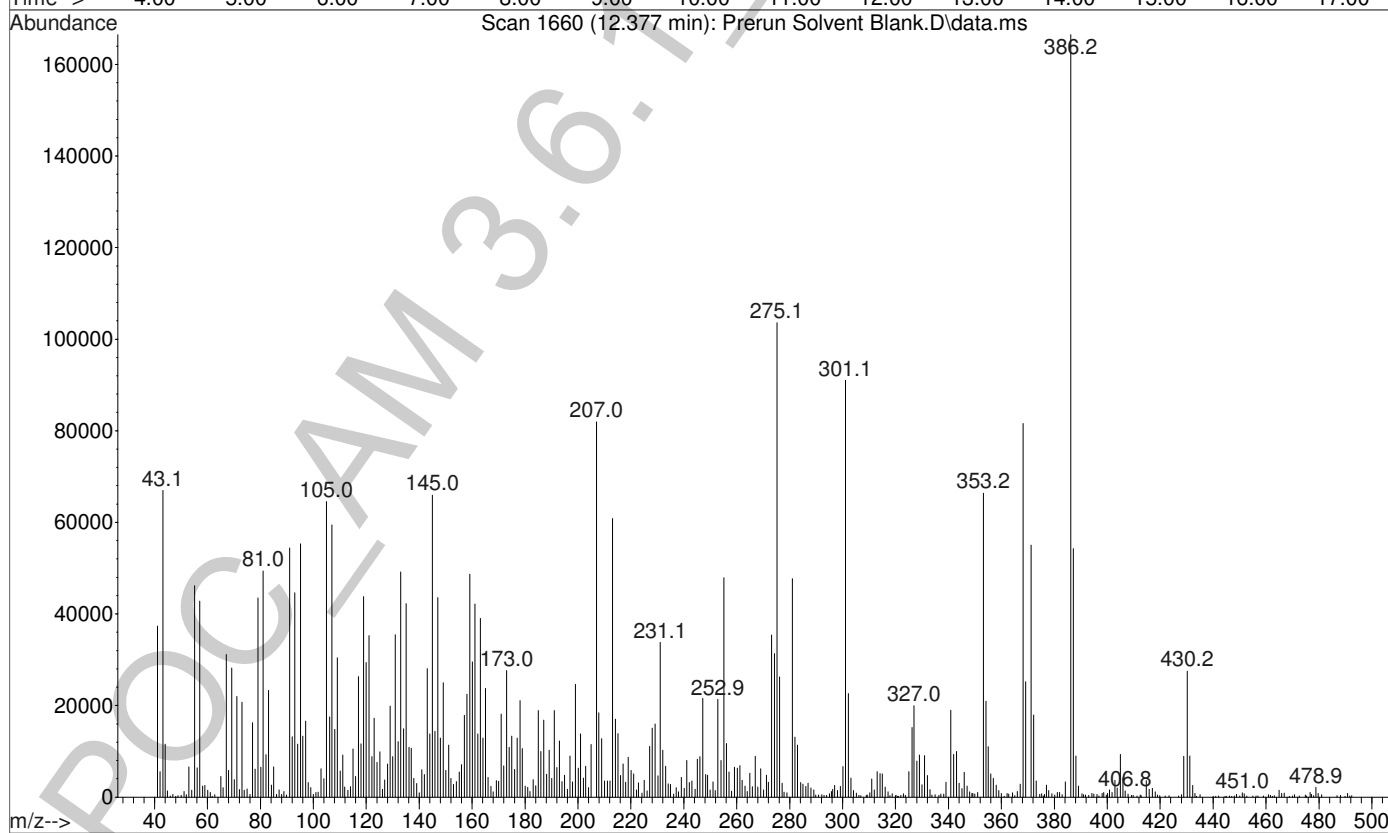
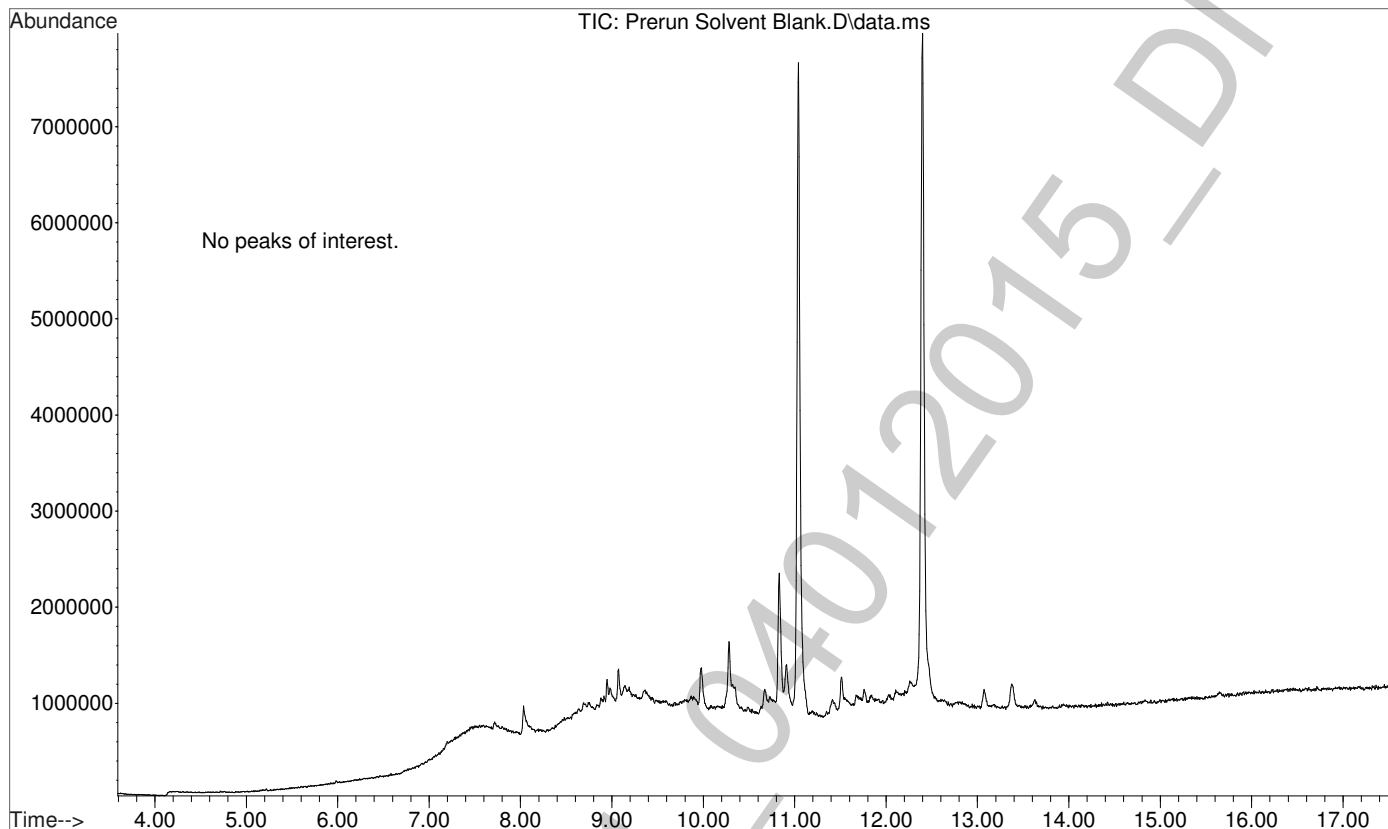


File :C:\gcms\1\data\Blood\040115BN\Negative Control-BN.D  
Operator : 5LAB-C01\ISPuser  
Acquired : 01 Apr 2015 23:09 using AcqMethod BNSB120510.M  
Instrument : Major Mass Spec  
Sample Name: Negative Control - Utak Lot B0130  
Misc Info : Analytical Method 3.6.1  
Vial Number: 1

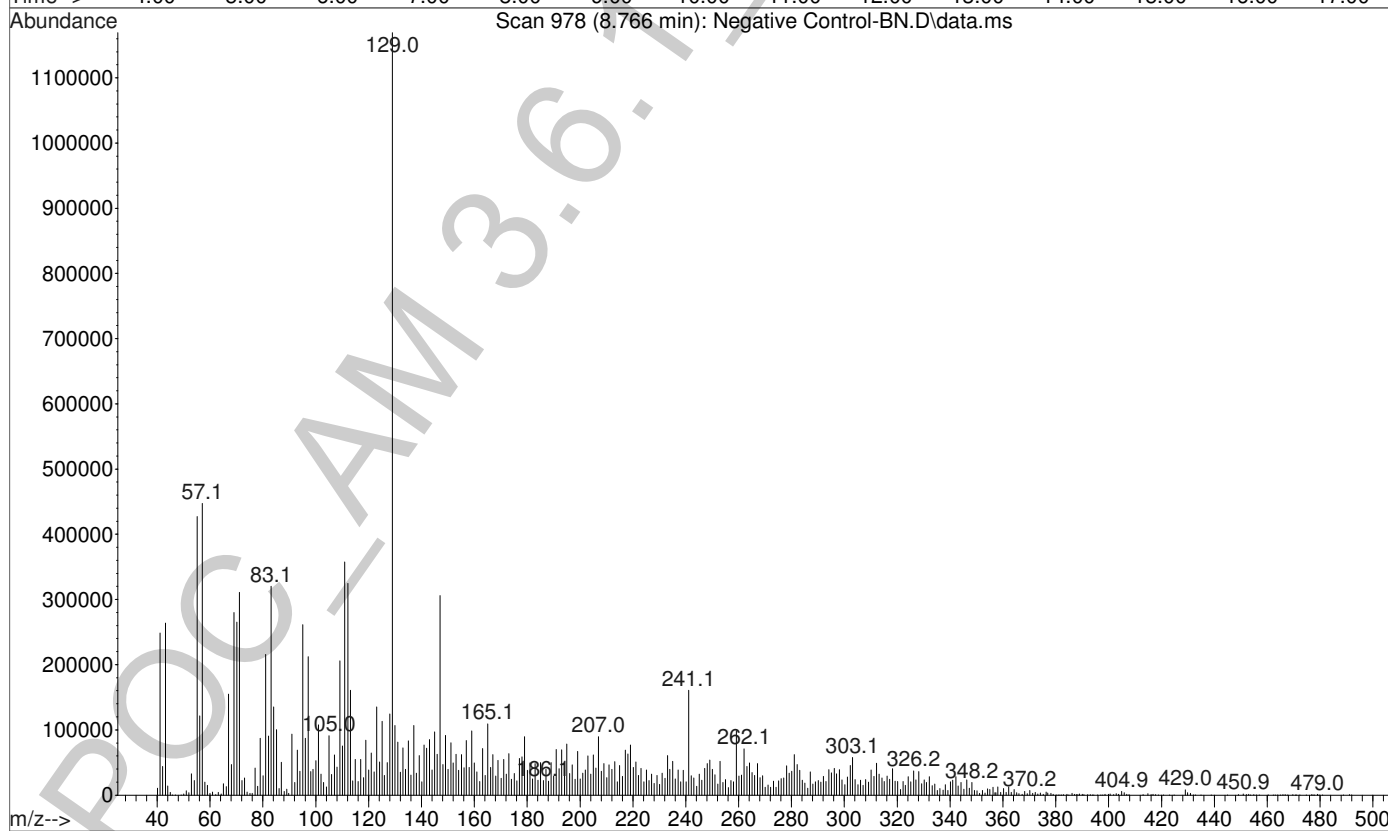
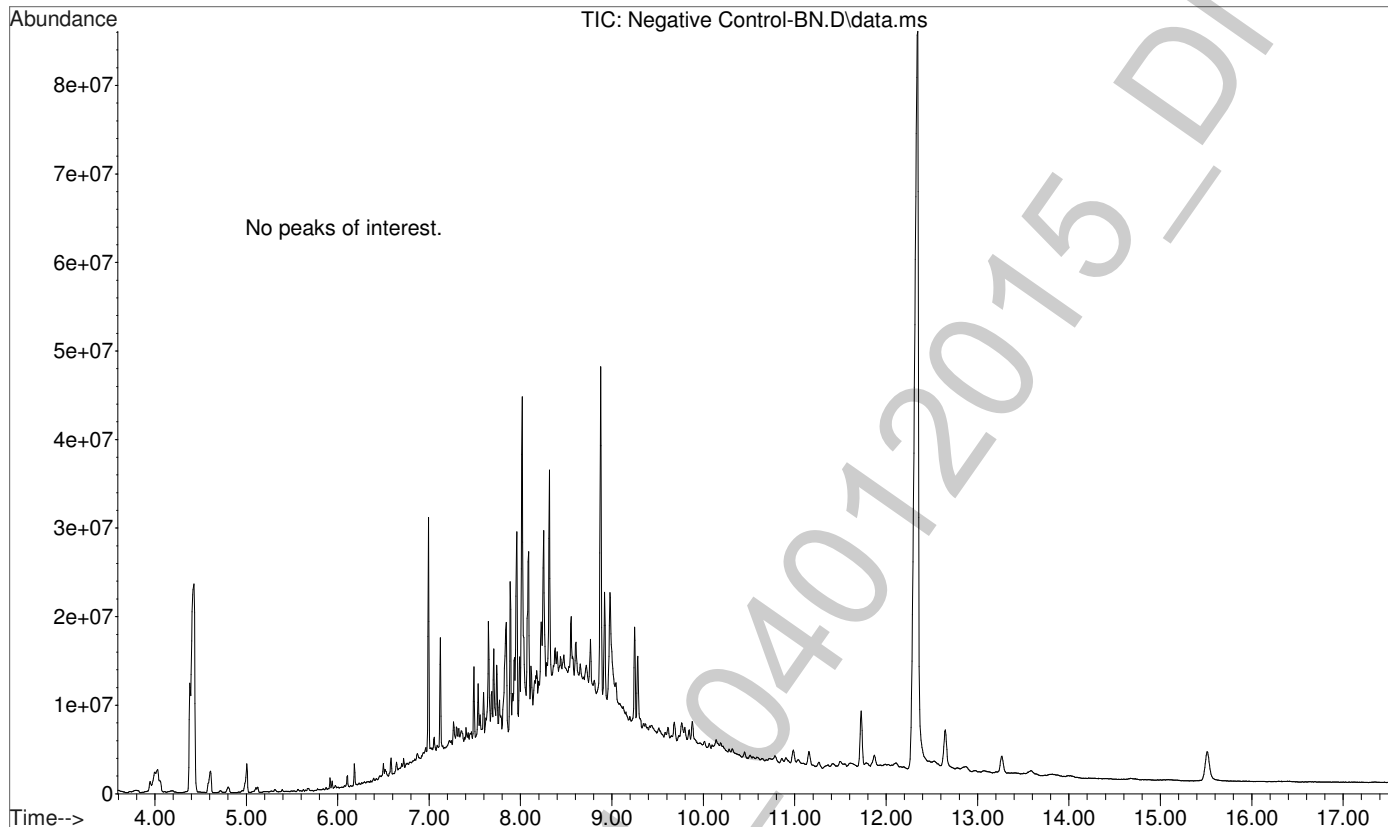





File :C:\gcms\1\data\Blood\040115BN\Negative Control-BN.D  
Operator : 5LAB-C01\ISPuser  
Acquired : 01 Apr 2015 23:09 using AcqMethod BNSB120510.M  
Instrument : Major Mass Spec  
Sample Name: Negative Control - Utak Lot B0130  
Misc Info : Analytical Method 3.6.1  
Vial Number: 1

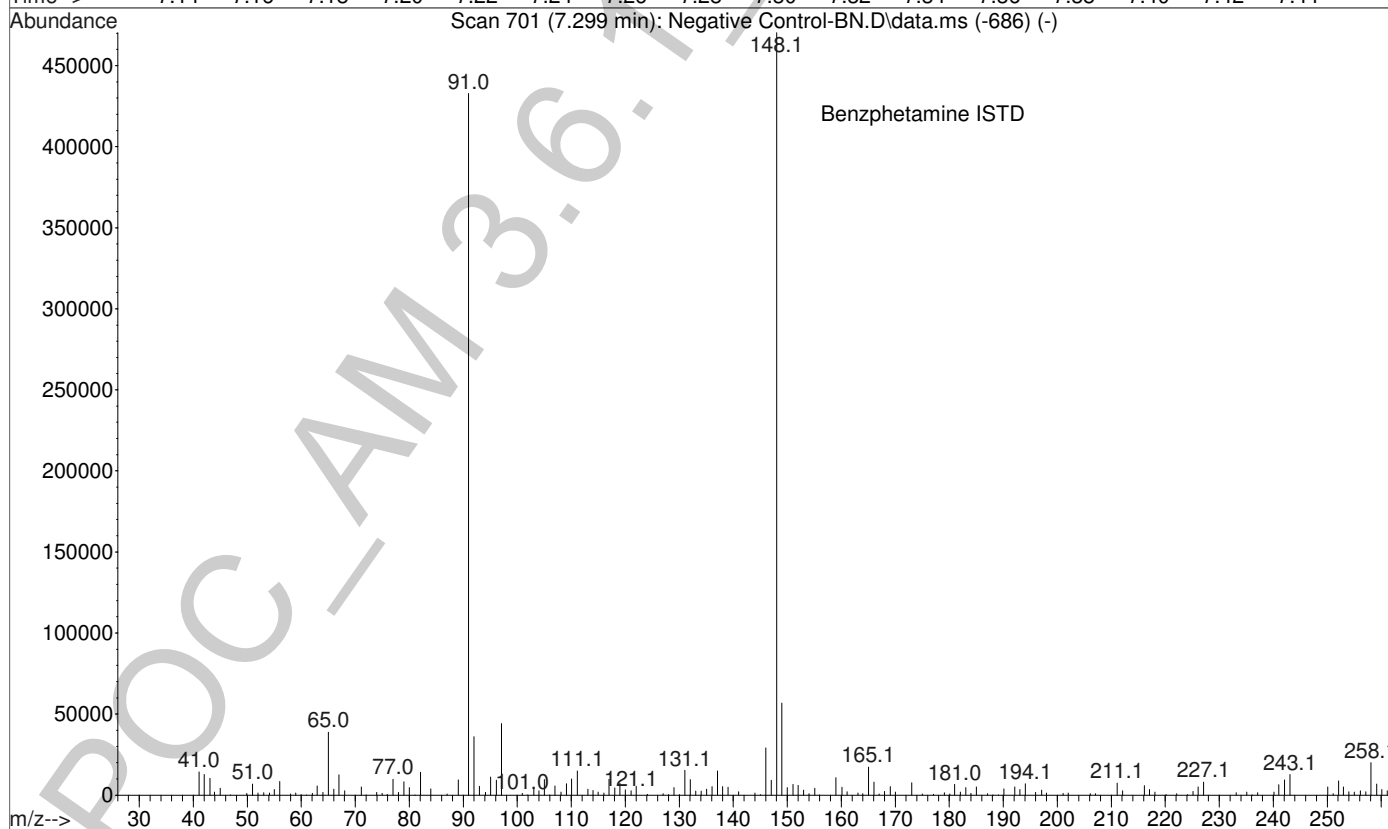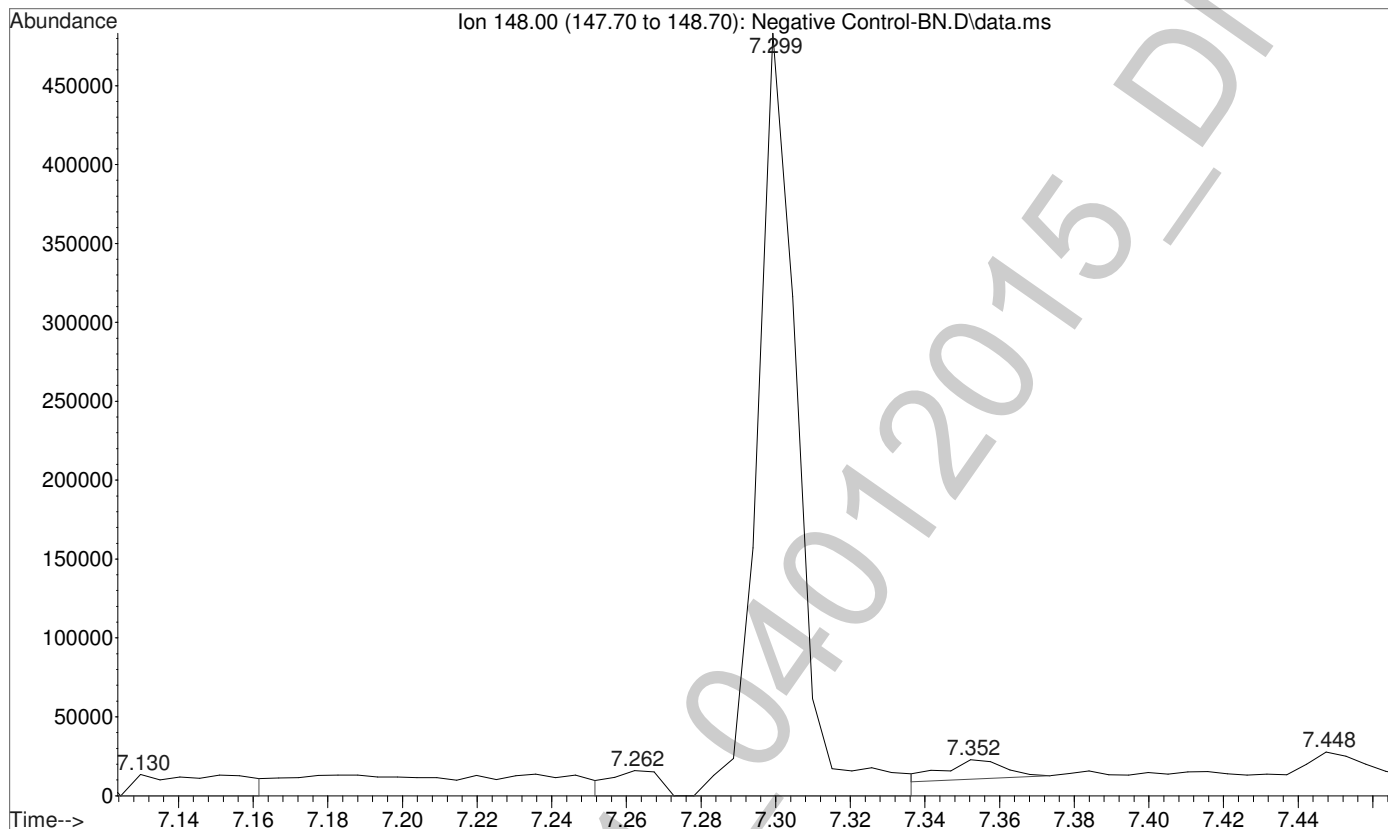



File :C:\gcms\1\data\Blood\040115BN\Negative Control-BN.D  
Operator : 5LAB-C01\ISPuser  
Acquired : 01 Apr 2015 23:09 using AcqMethod BNSB120510.M  
Instrument : Major Mass Spec  
Sample Name: Negative Control - Utak Lot B0130  
Misc Info : Analytical Method 3.6.1  
Vial Number: 1

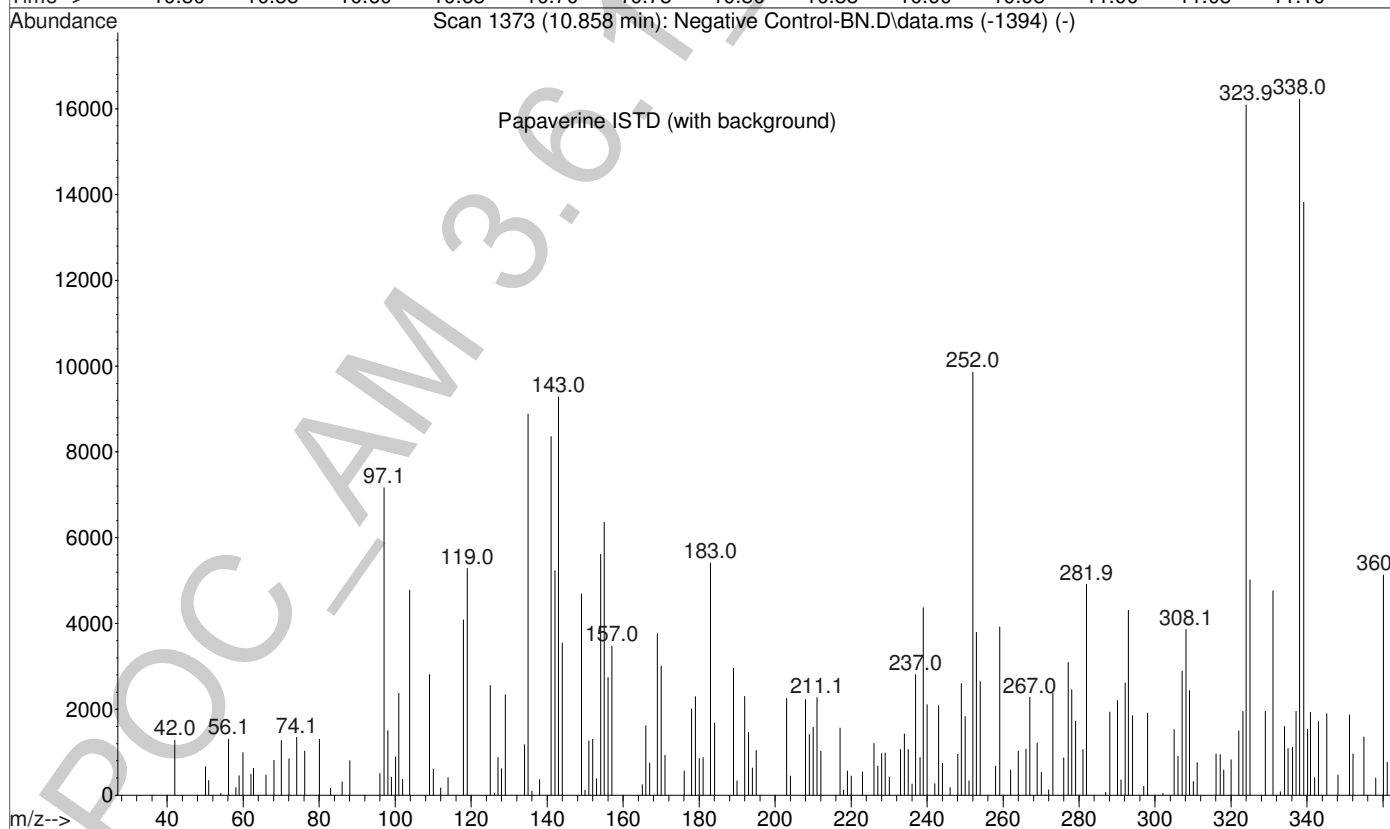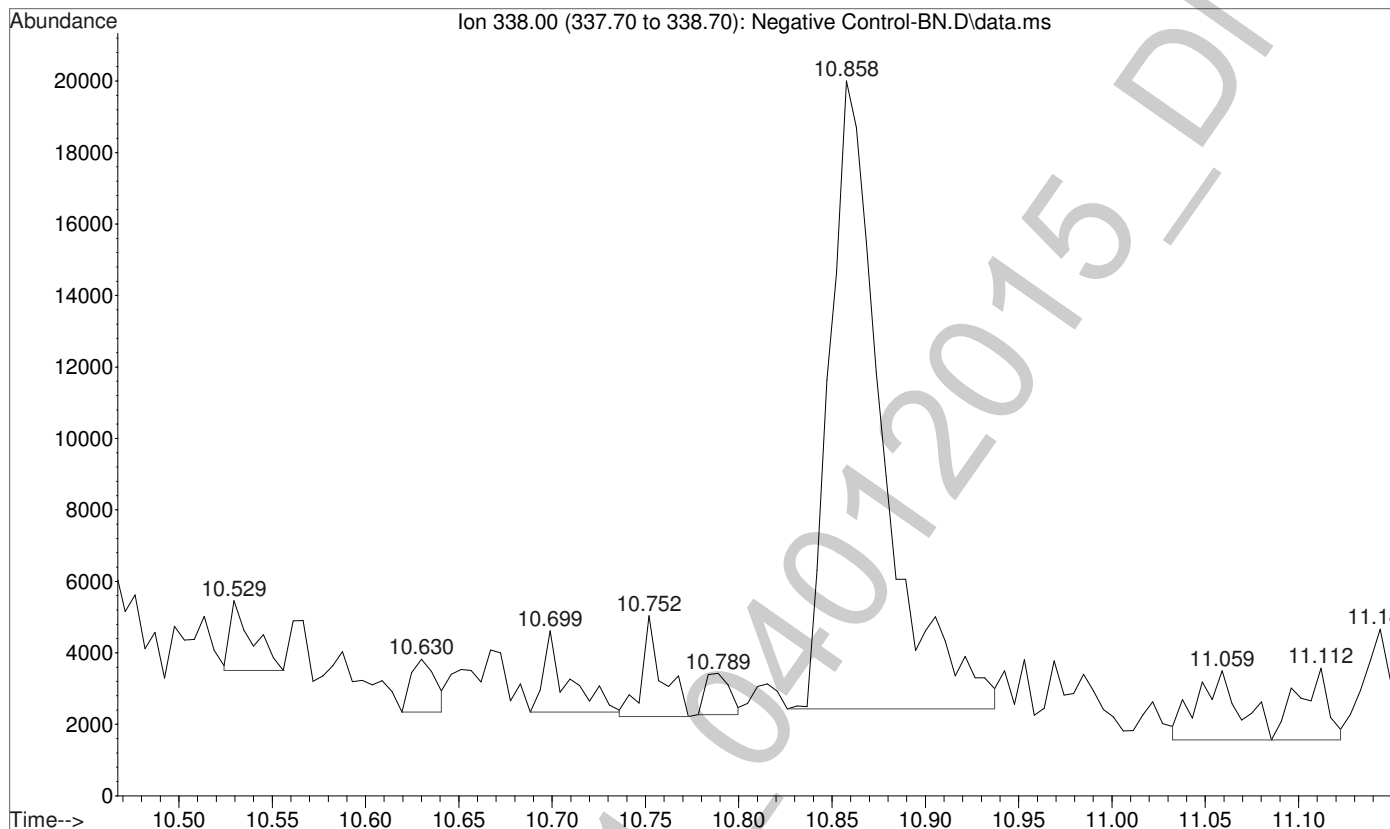



File :C:\gcms\1\data\Blood\040115BN\Spiked Positive Control-BN.D  
Operator : 5LAB-C01\ISPuser  
Acquired : 01 Apr 2015 23:32 using AcqMethod BNSB120510.M  
Instrument : Major Mass Spec  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1  
Vial Number: 2

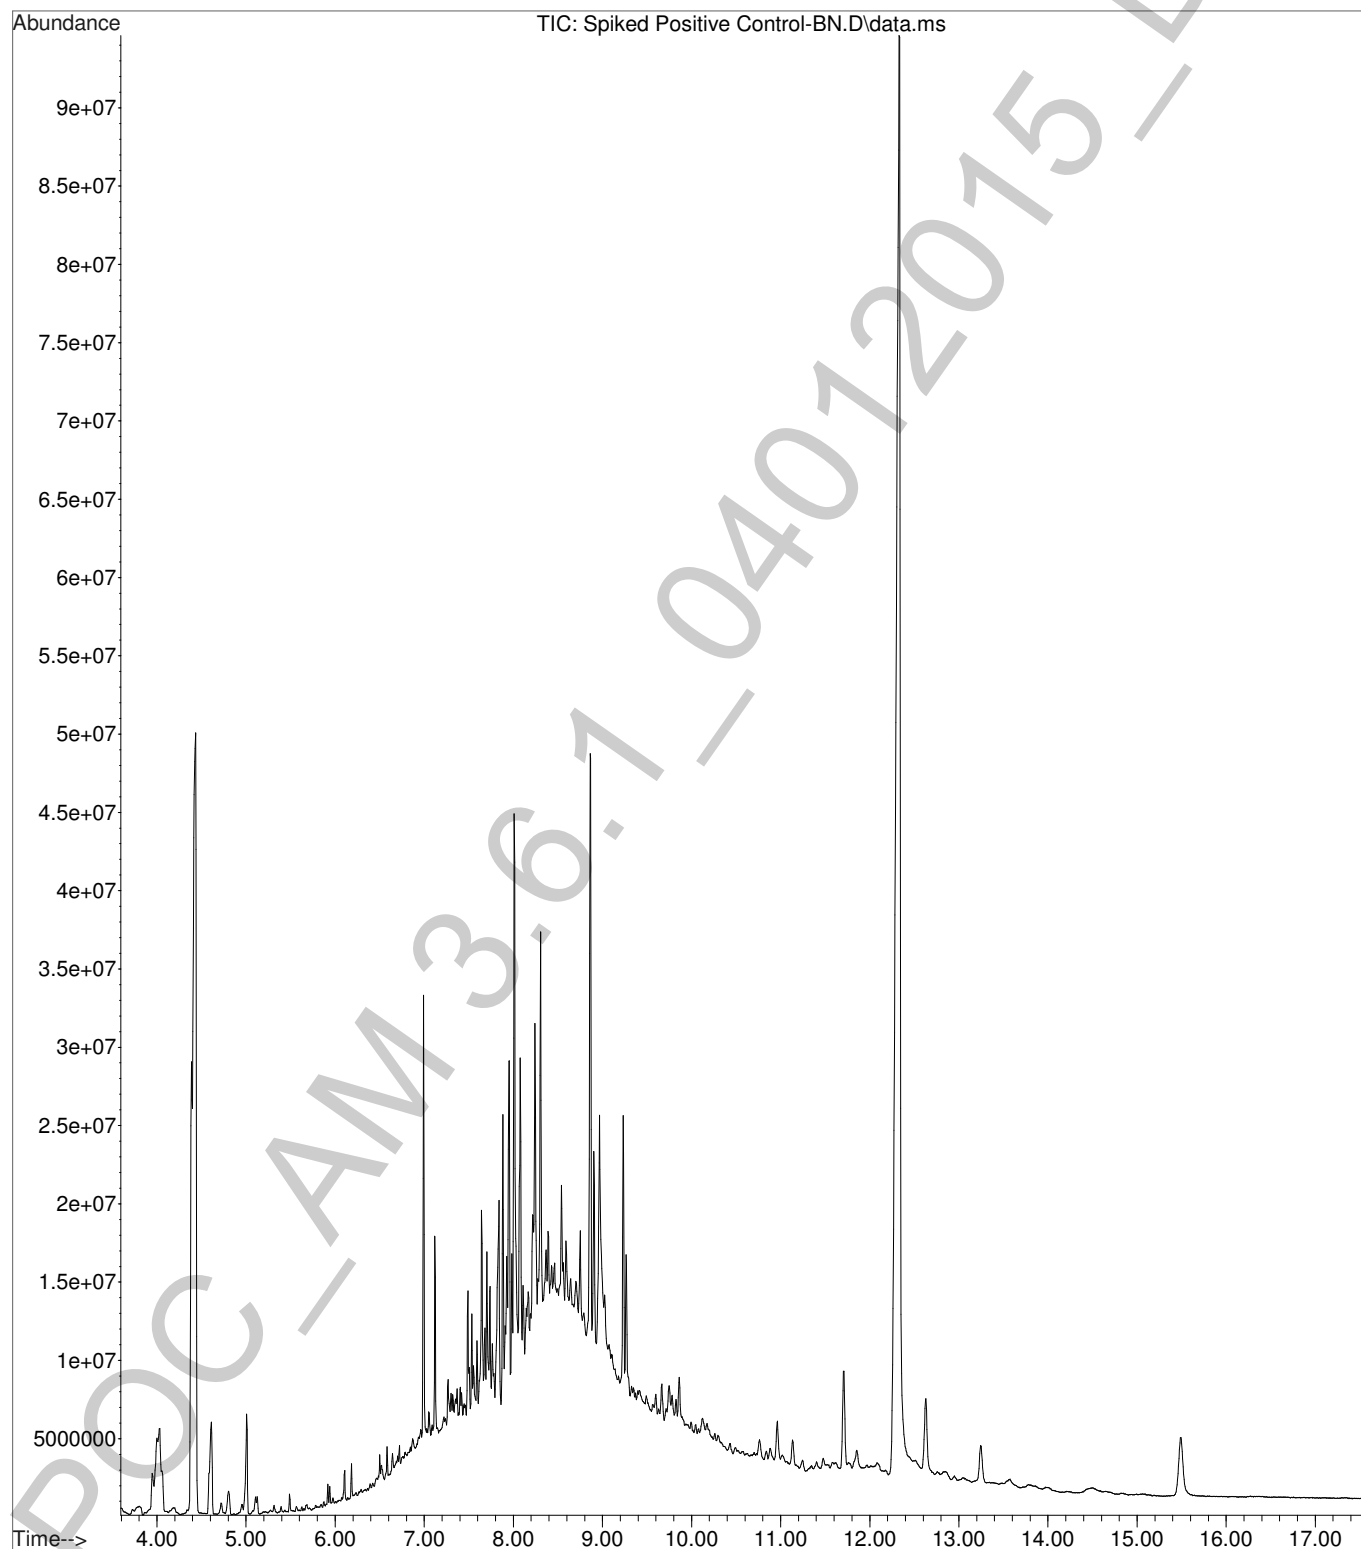



File :C:\gcms\1\data\Blood\040115BN\Spiked Positive Control-BN.D  
Operator : 5LAB-C01\ISPuser  
Acquired : 01 Apr 2015 23:32 using AcqMethod BNSB120510.M  
Instrument : Major Mass Spec  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1  
Vial Number: 2

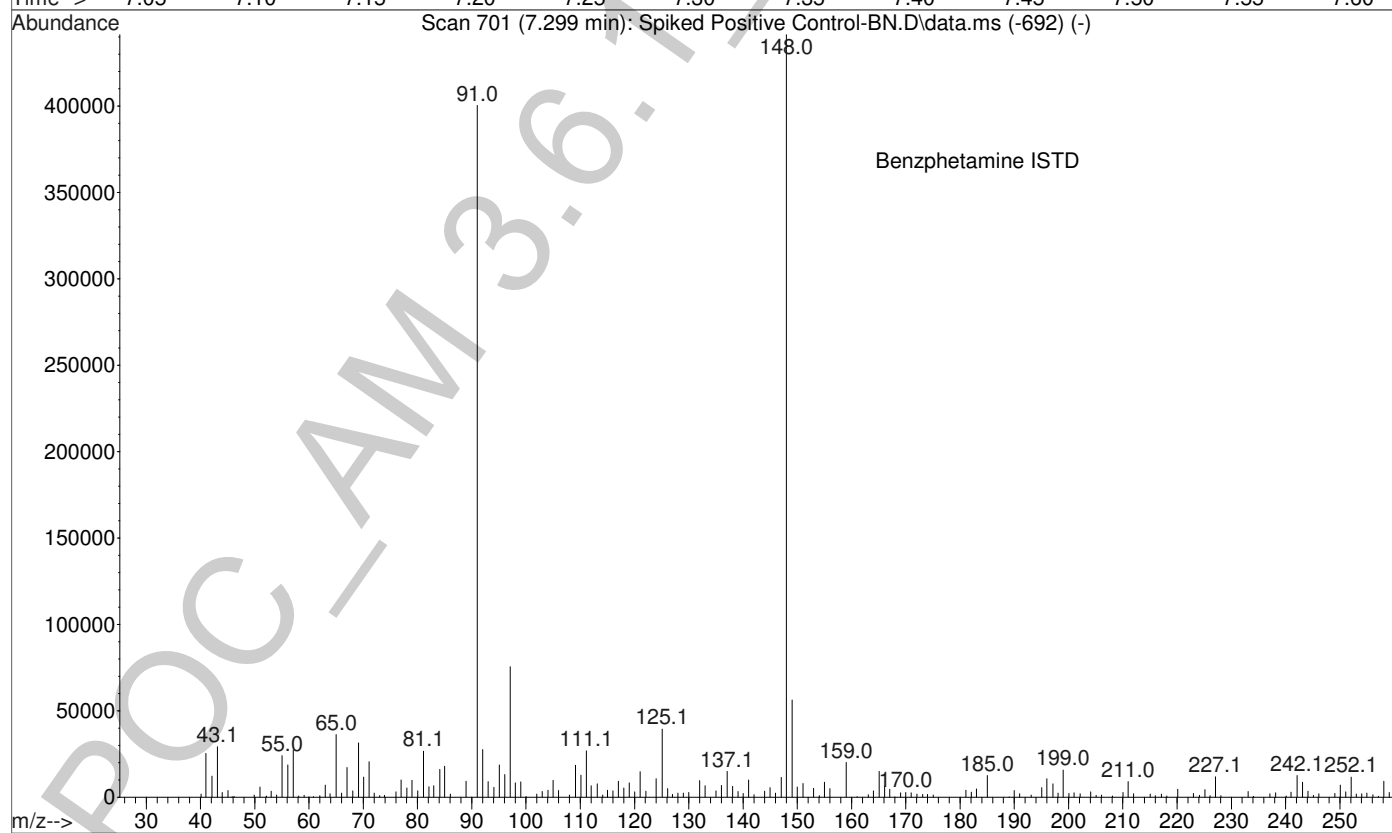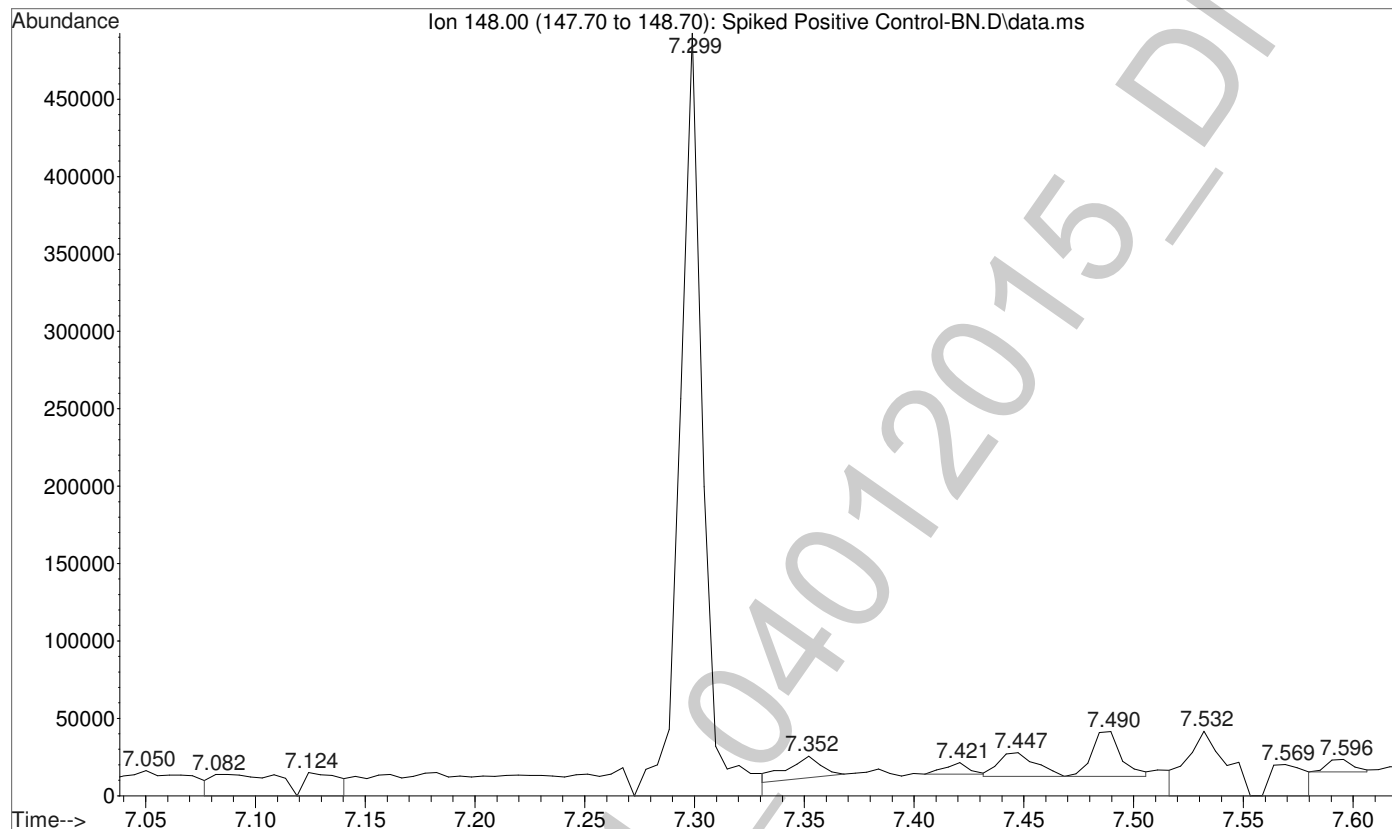



File :C:\gcms\1\data\Blood\040115BN\Spiked Positive Control-BN.D  
Operator : 5LAB-C01\ISPuser  
Acquired : 01 Apr 2015 23:32 using AcqMethod BNSB120510.M  
Instrument : Major Mass Spec  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1  
Vial Number: 2

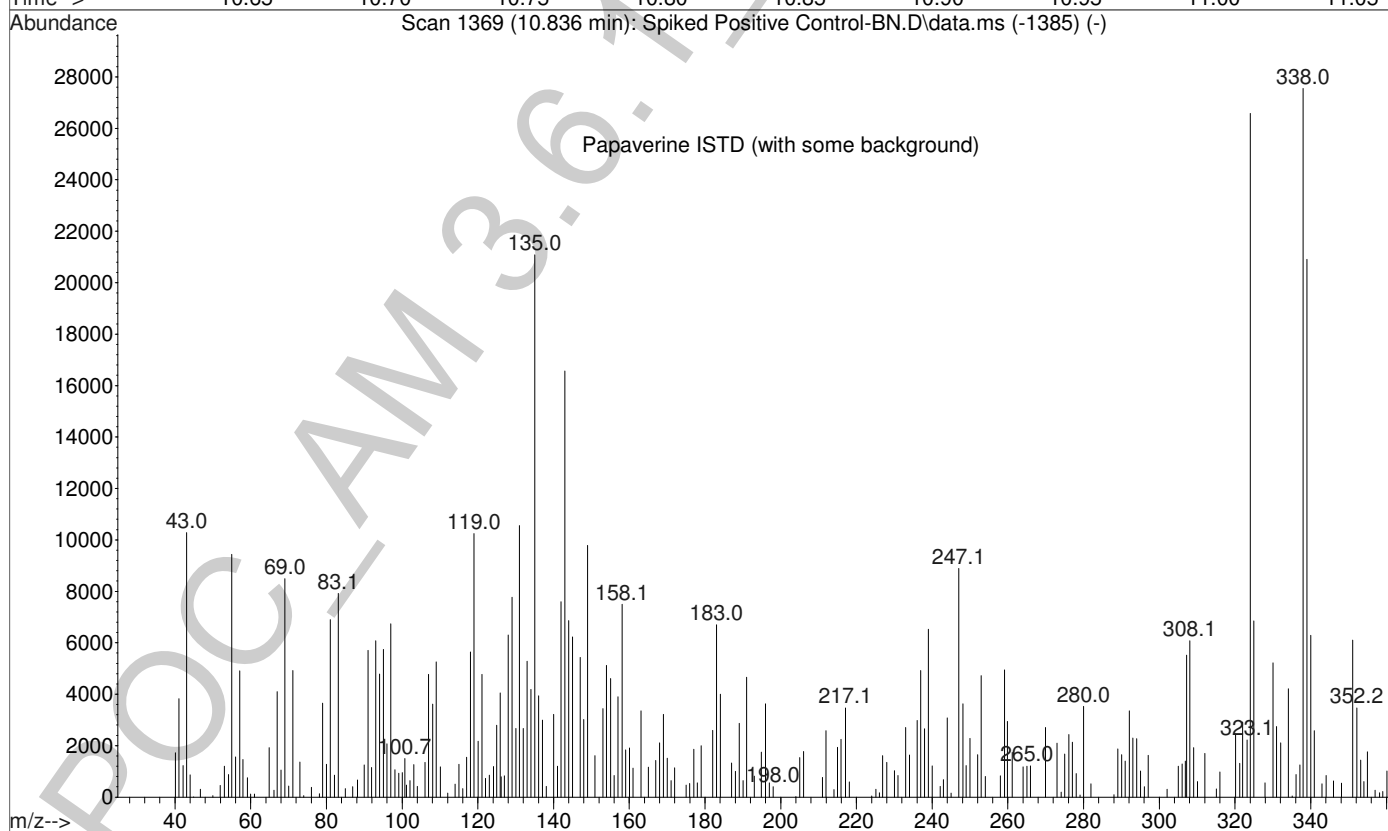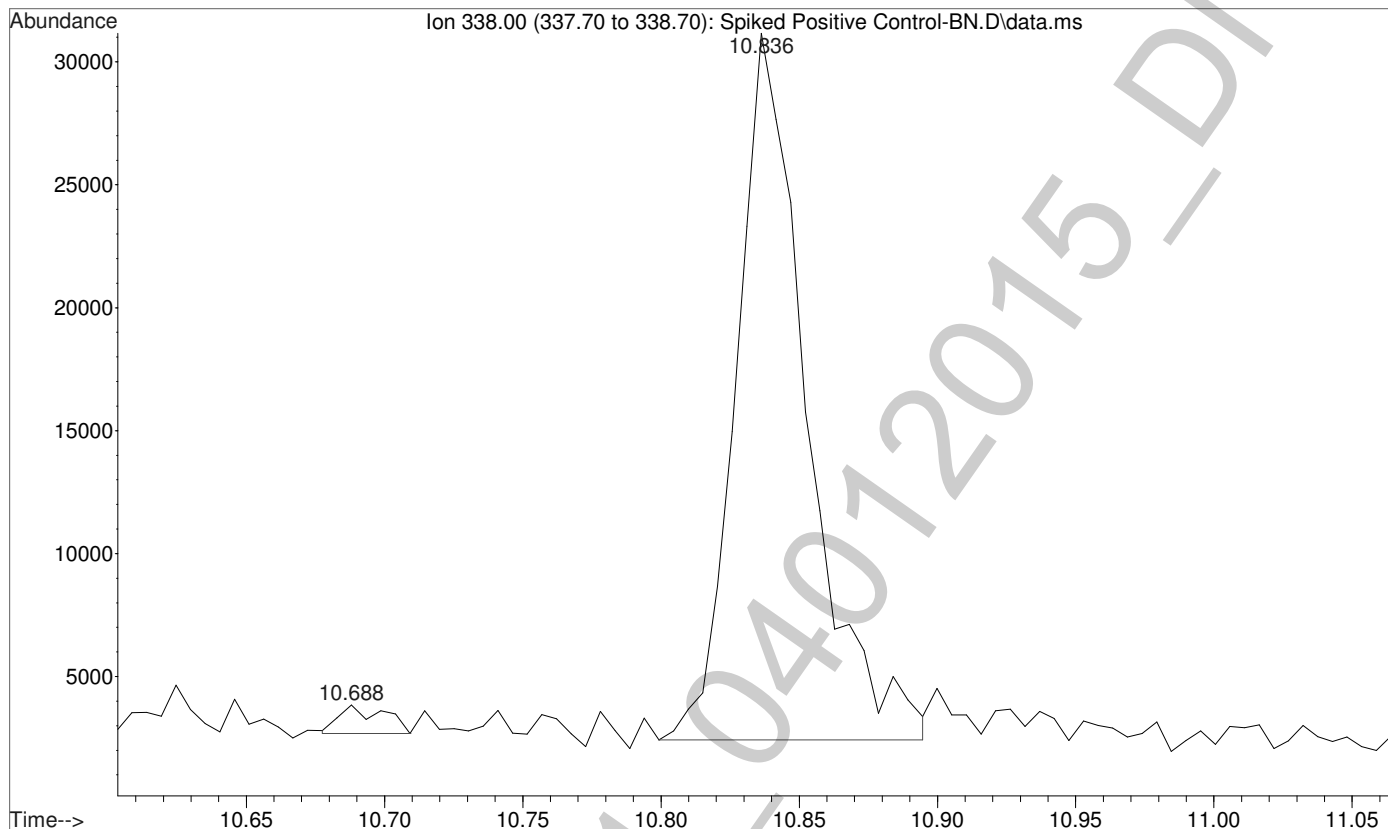



File :C:\gcms\1\data\Blood\040115BN\Spiked Positive Control-BN.D  
Operator : 5LAB-C01\ISPuser  
Acquired : 01 Apr 2015 23:32 using AcqMethod BNSB120510.M  
Instrument : Major Mass Spec  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1  
Vial Number: 2

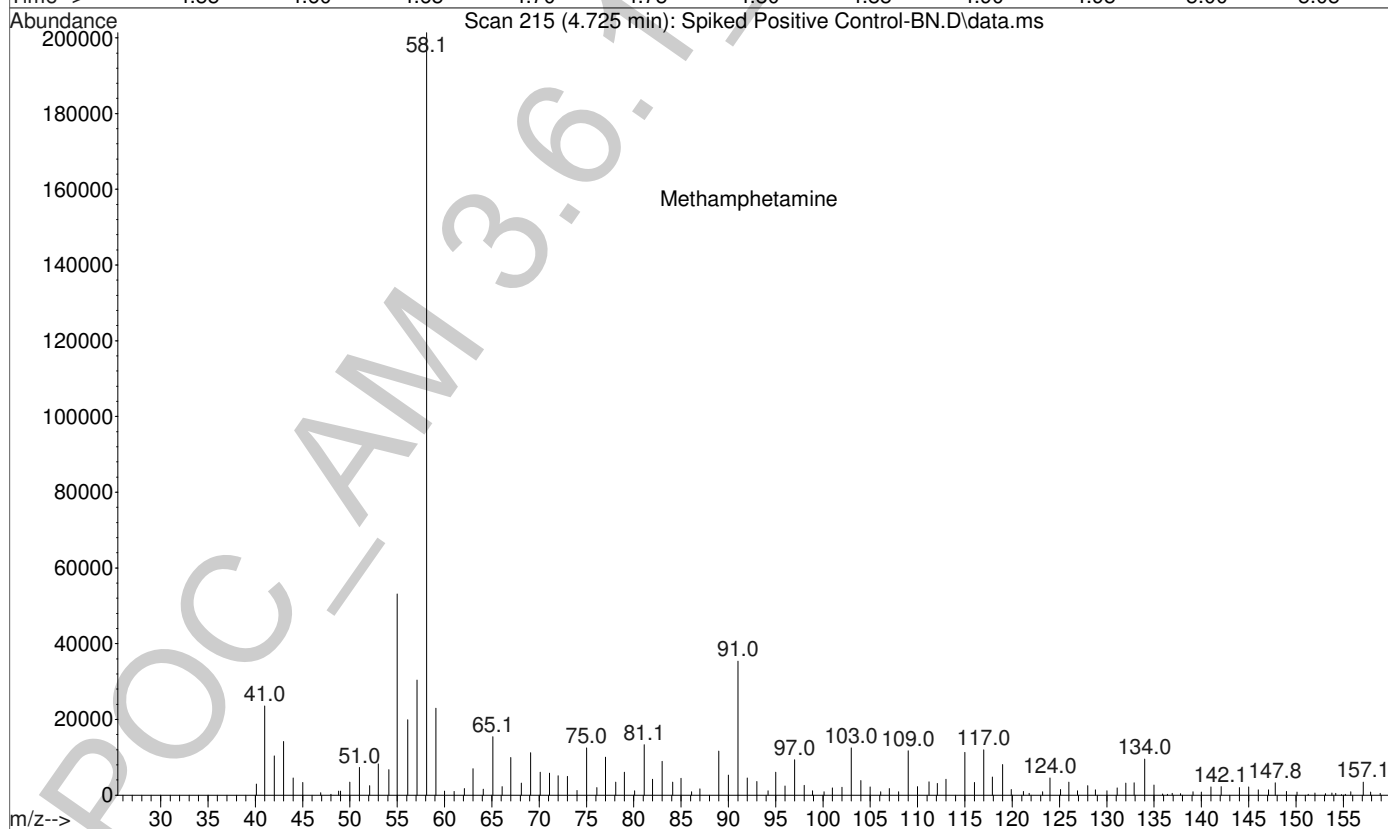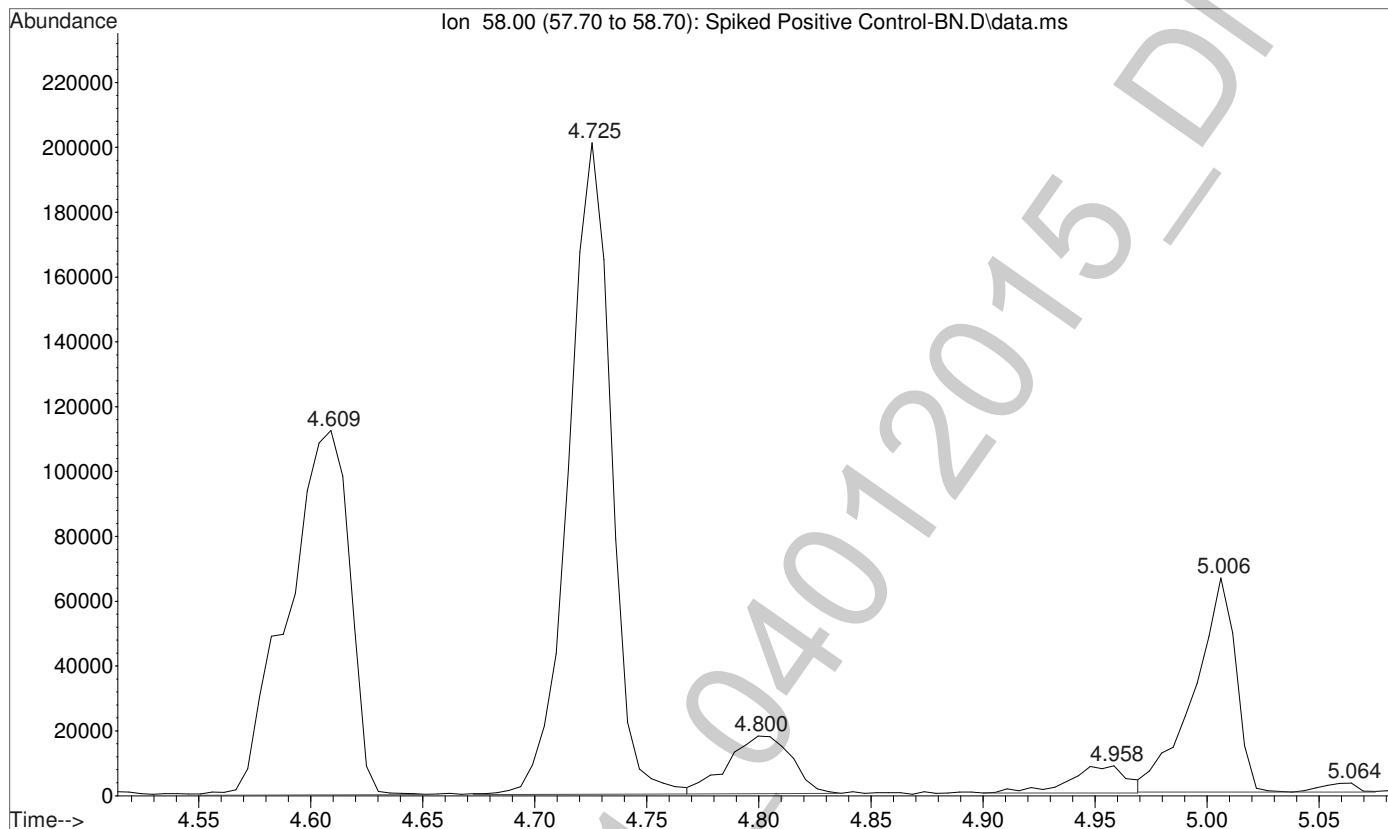

File :C:\gcms\1\data\Blood\040115BN\Spiked Positive Control-BN.D  
Operator : 5LAB-C01\ISPuser  
Acquired : 01 Apr 2015 23:32 using AcqMethod BNSB120510.M  
Instrument : Major Mass Spec  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1  
Vial Number: 2

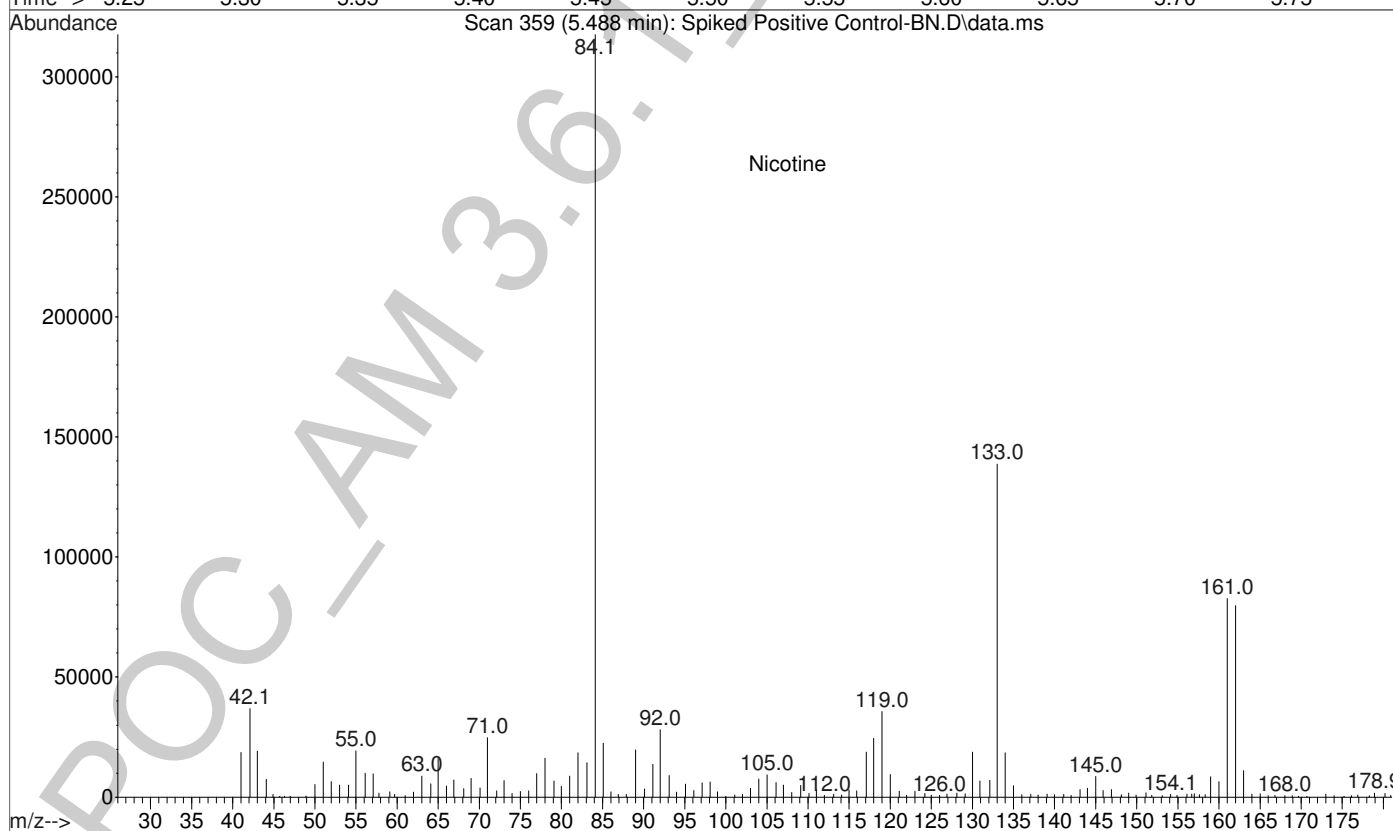
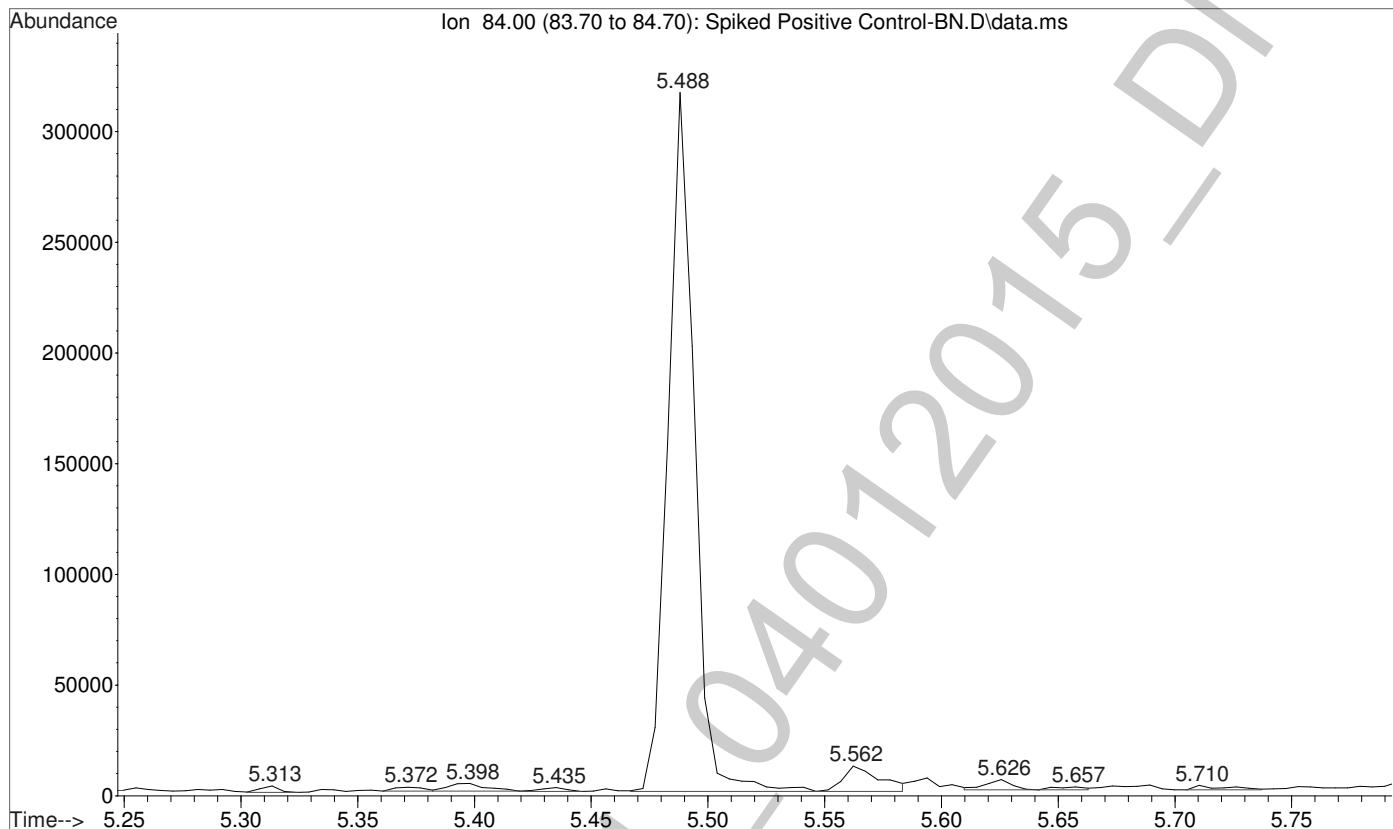


File :C:\gcms\1\data\Blood\040115BN\Spiked Positive Control-BN.D  
Operator : 5LAB-C01\ISPuser  
Acquired : 01 Apr 2015 23:32 using AcqMethod BNSB120510.M  
Instrument : Major Mass Spec  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1  
Vial Number: 2

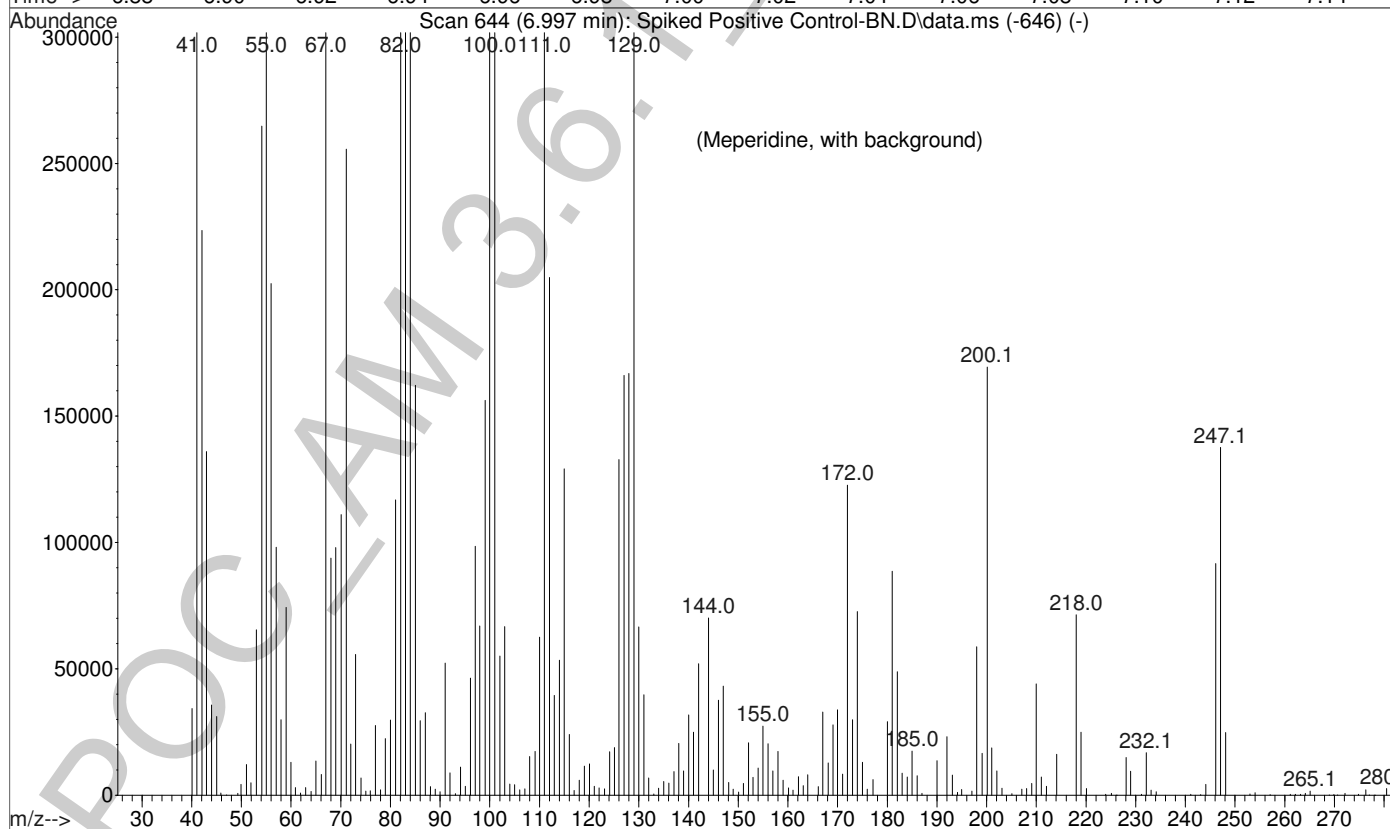
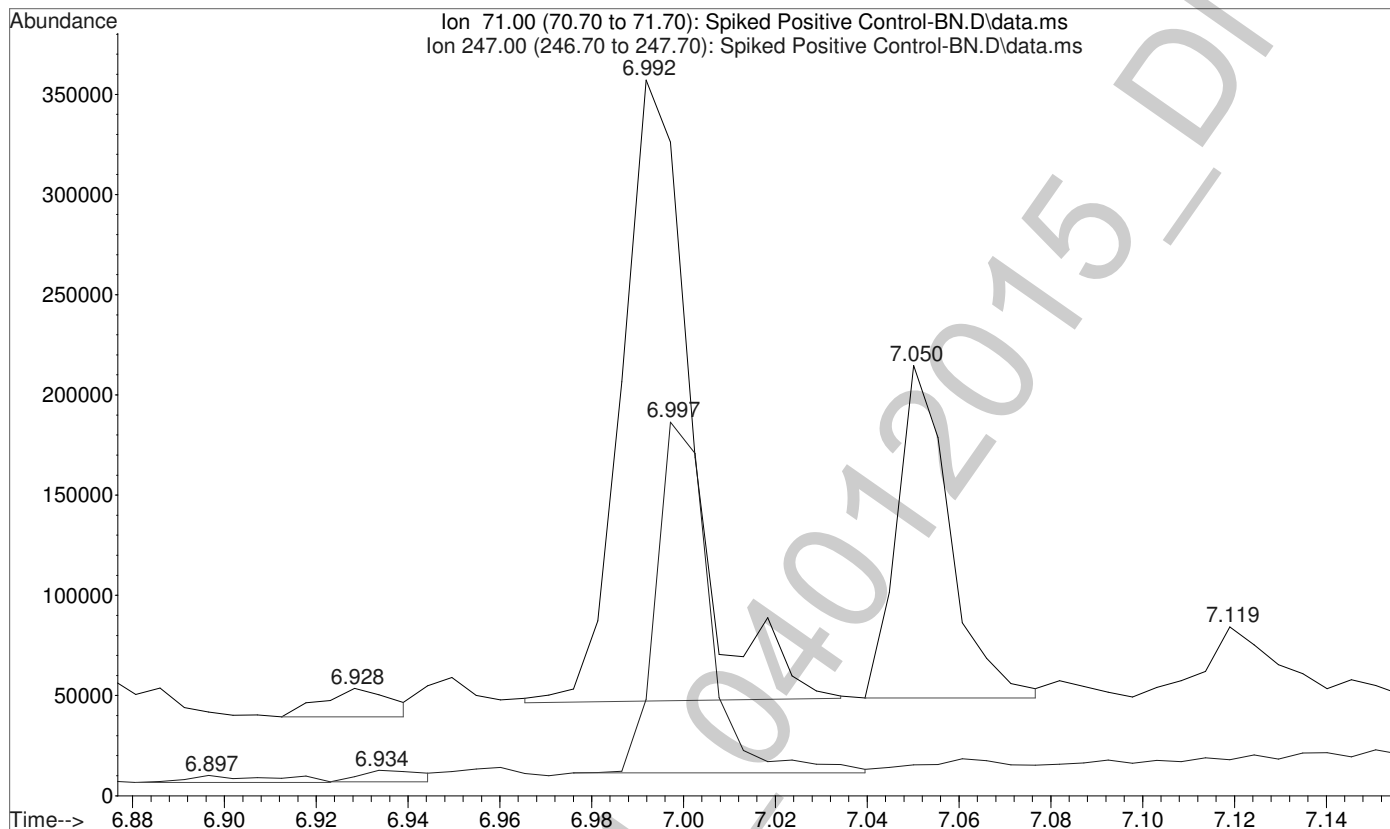






File :C:\gcms\1\data\Blood\040115BN\Spiked Positive Control-BN.D  
Operator : 5LAB-C01\ISPuser  
Acquired : 01 Apr 2015 23:32 using AcqMethod BNSB120510.M  
Instrument : Major Mass Spec  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1  
Vial Number: 2

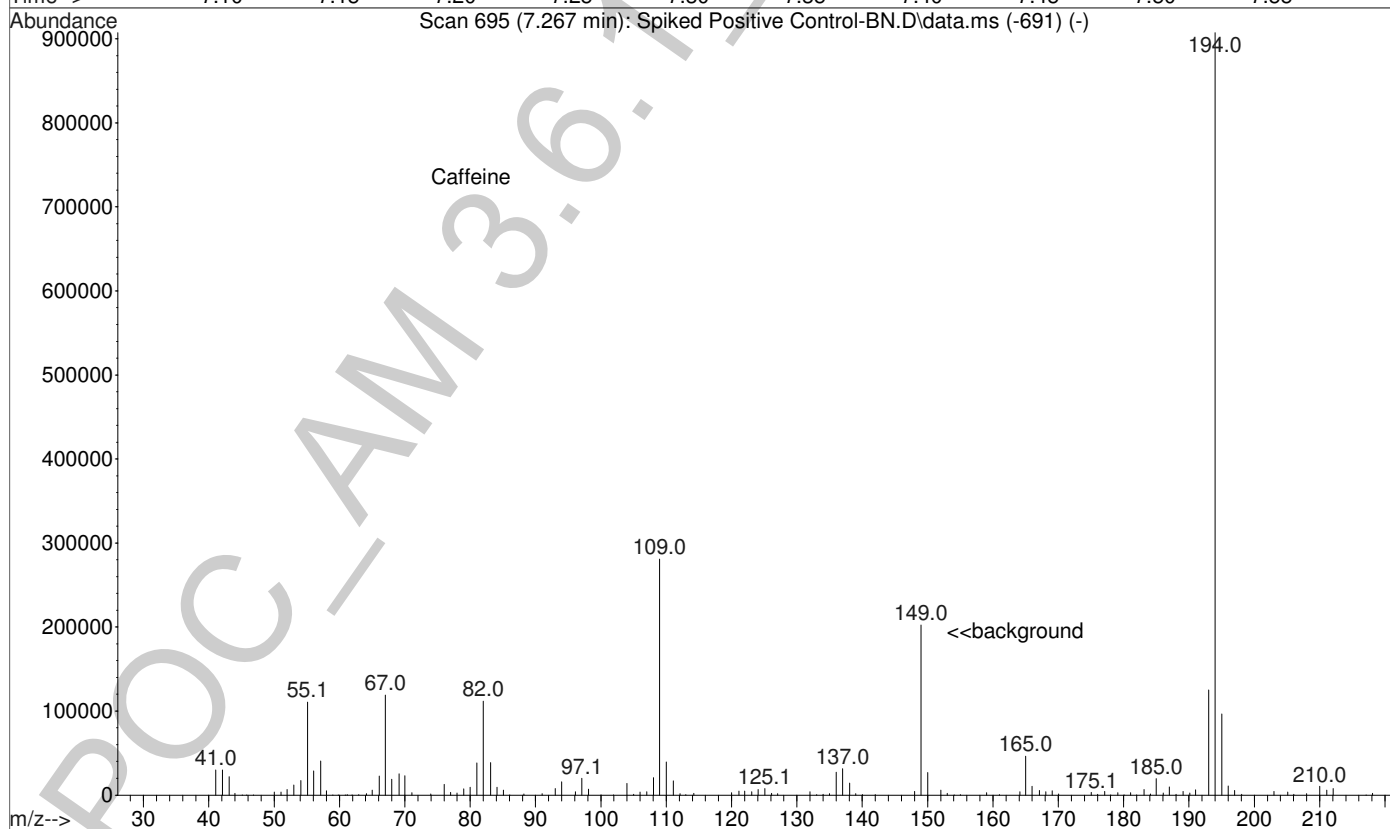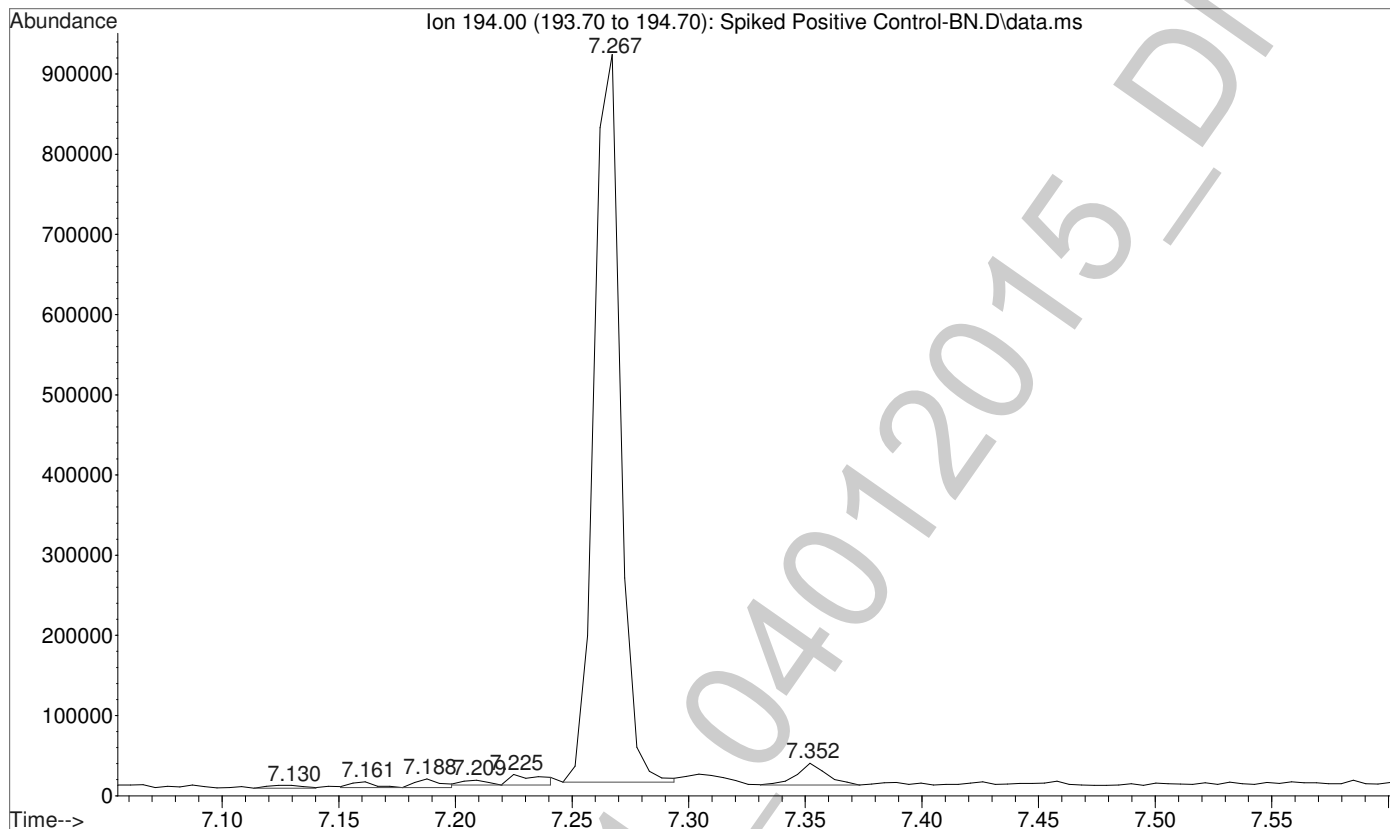



File :C:\gcms\1\data\Blood\040115BN\Spiked Positive Control-BN.D  
Operator : 5LAB-C01\ISPuser  
Acquired : 01 Apr 2015 23:32 using AcqMethod BNSB120510.M  
Instrument : Major Mass Spec  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1  
Vial Number: 2

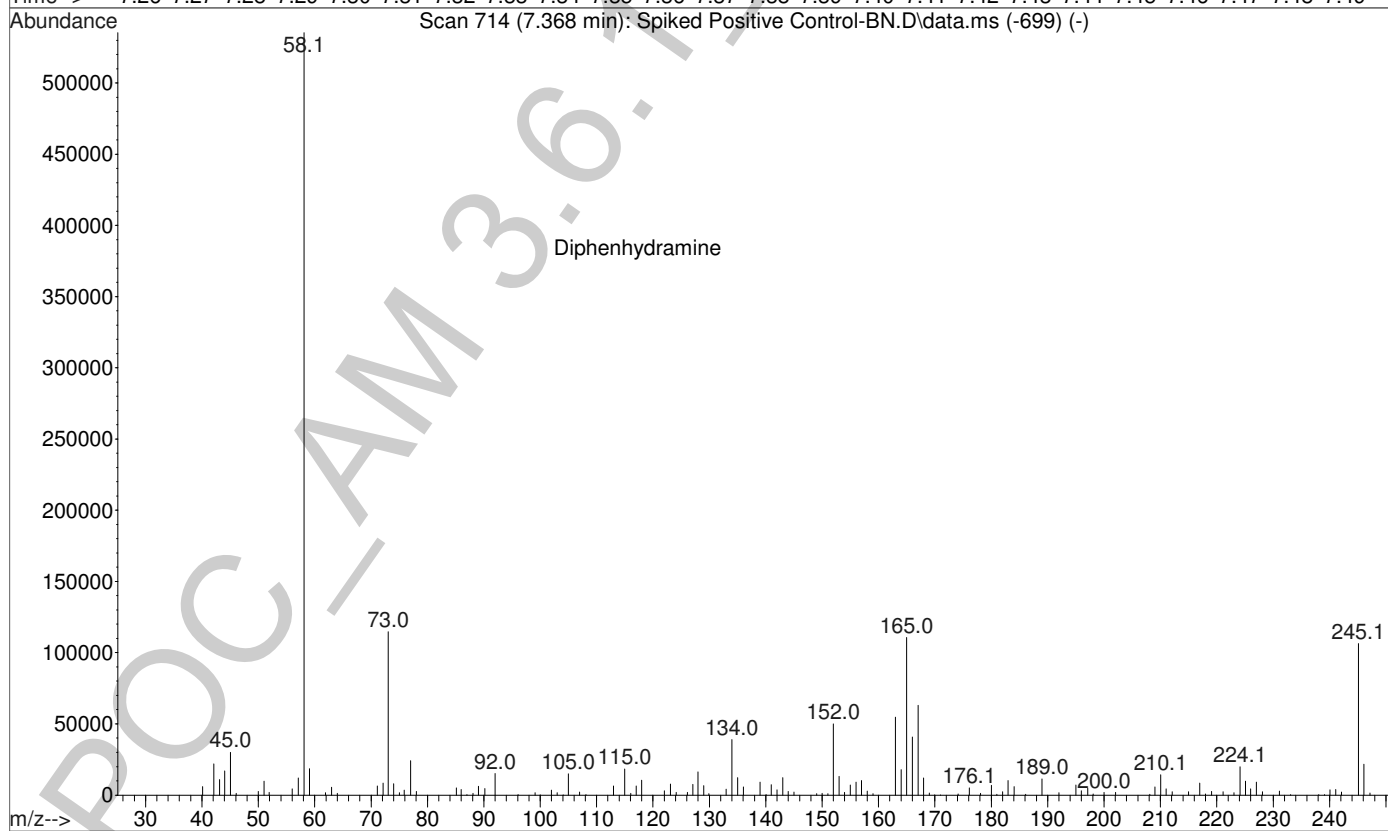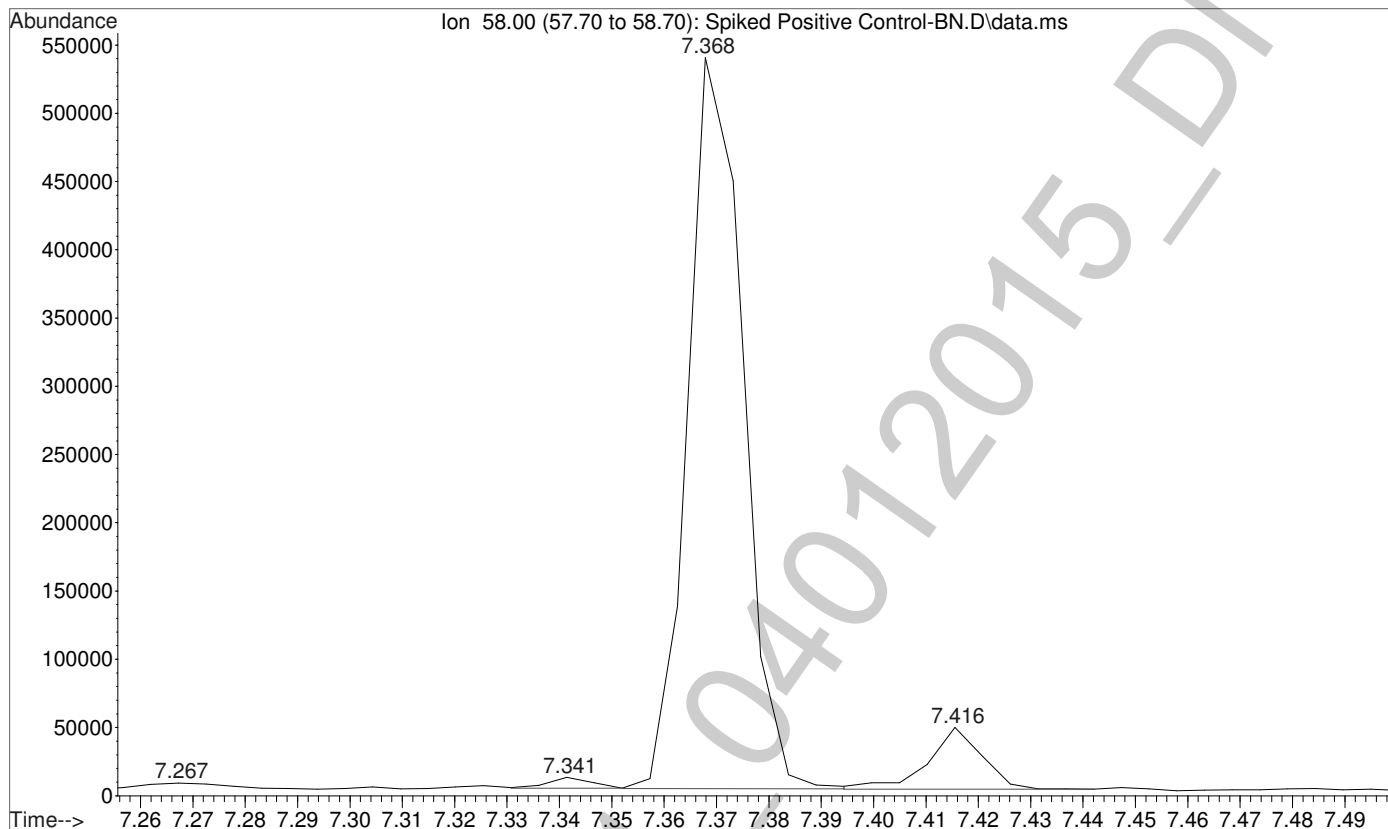



File :C:\gcms\1\data\Blood\040115BN\Spiked Positive Control-BN.D  
Operator : 5LAB-C01\ISPuser  
Acquired : 01 Apr 2015 23:32 using AcqMethod BNSB120510.M  
Instrument : Major Mass Spec  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1  
Vial Number: 2

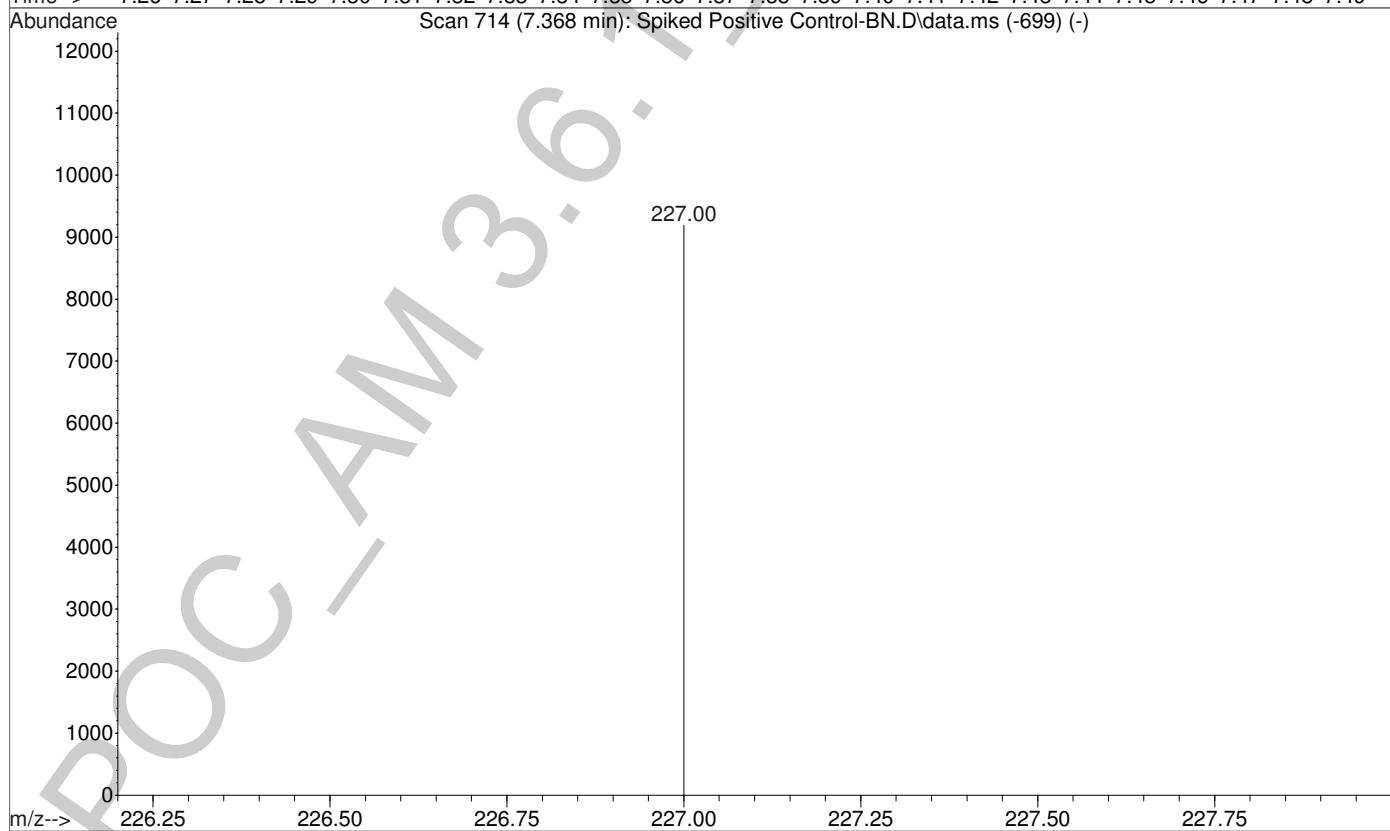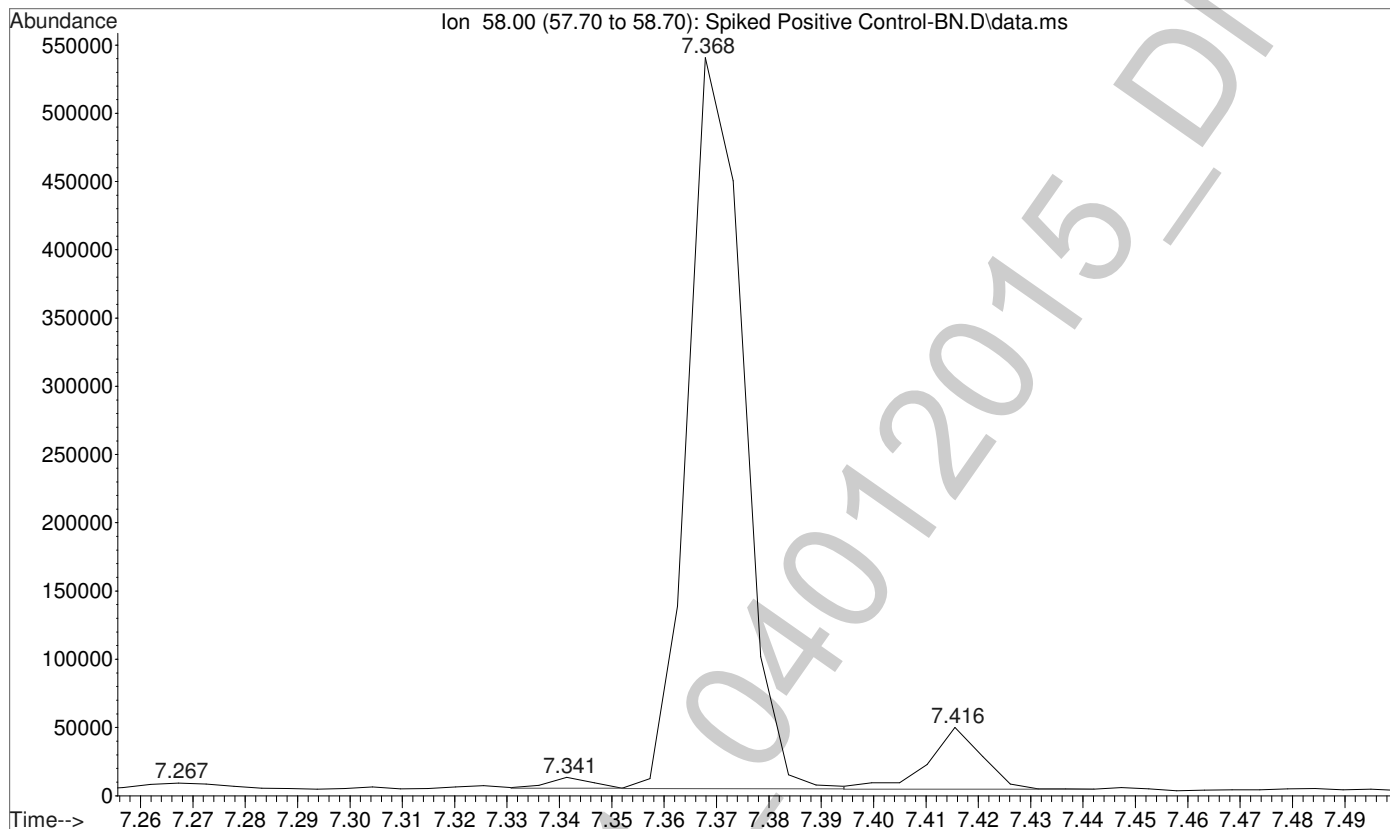



File :C:\gcms\1\data\Blood\040115BN\Spiked Positive Control-BN.D  
Operator : 5LAB-C01\ISPuser  
Acquired : 01 Apr 2015 23:32 using AcqMethod BNSB120510.M  
Instrument : Major Mass Spec  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1  
Vial Number: 2

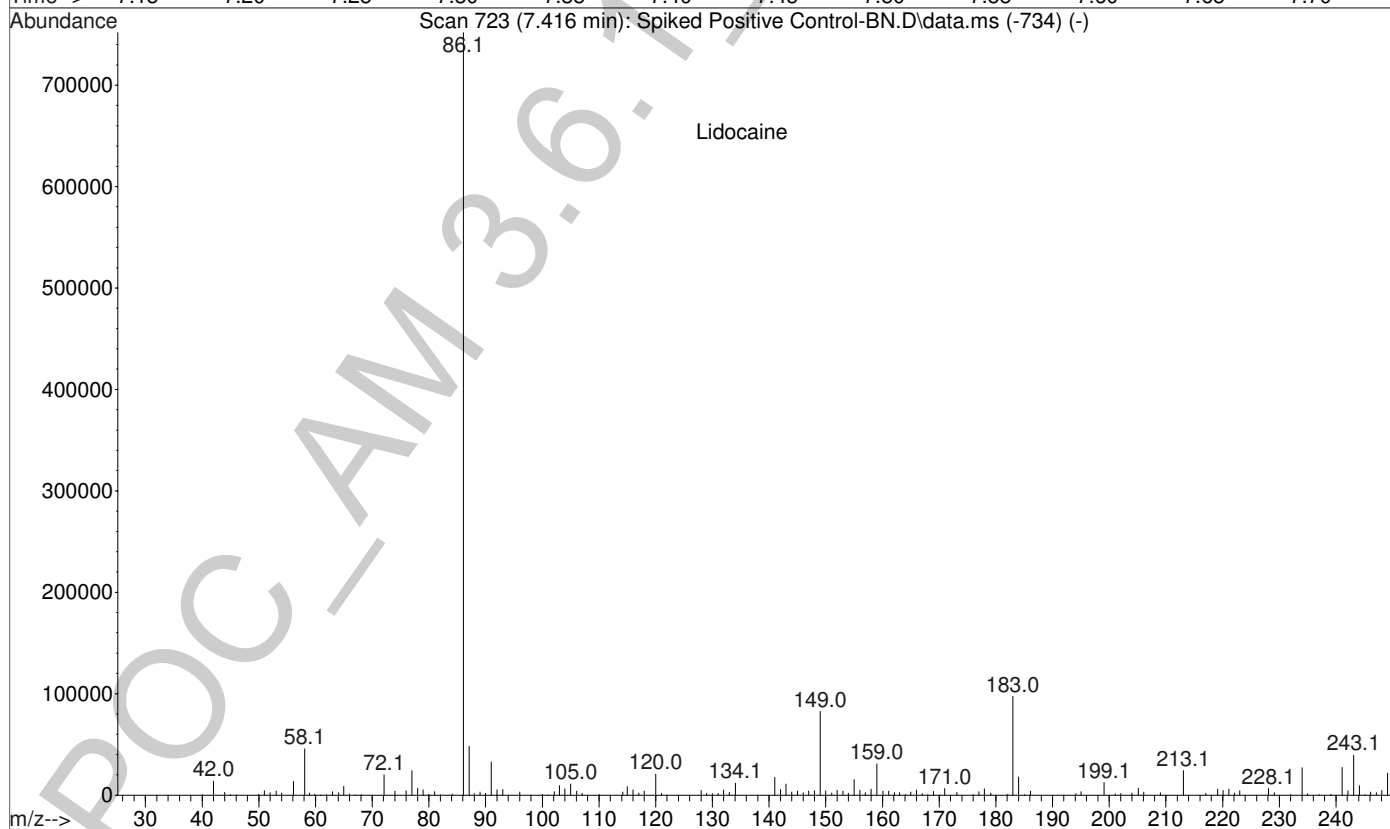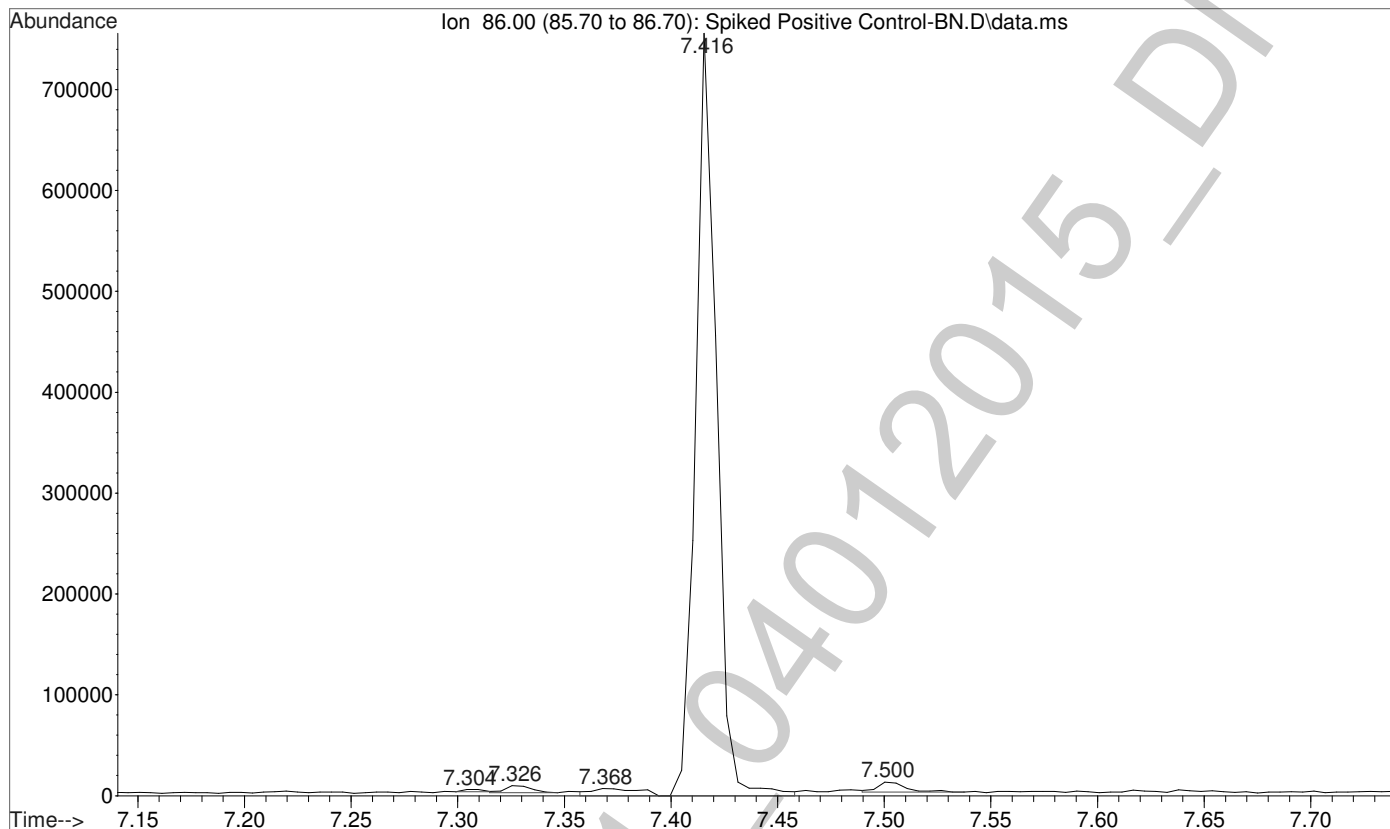



File :C:\gcms\1\data\Blood\040115BN\Spiked Positive Control-BN.D  
Operator : 5LAB-C01\ISPuser  
Acquired : 01 Apr 2015 23:32 using AcqMethod BNSB120510.M  
Instrument : Major Mass Spec  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1  
Vial Number: 2

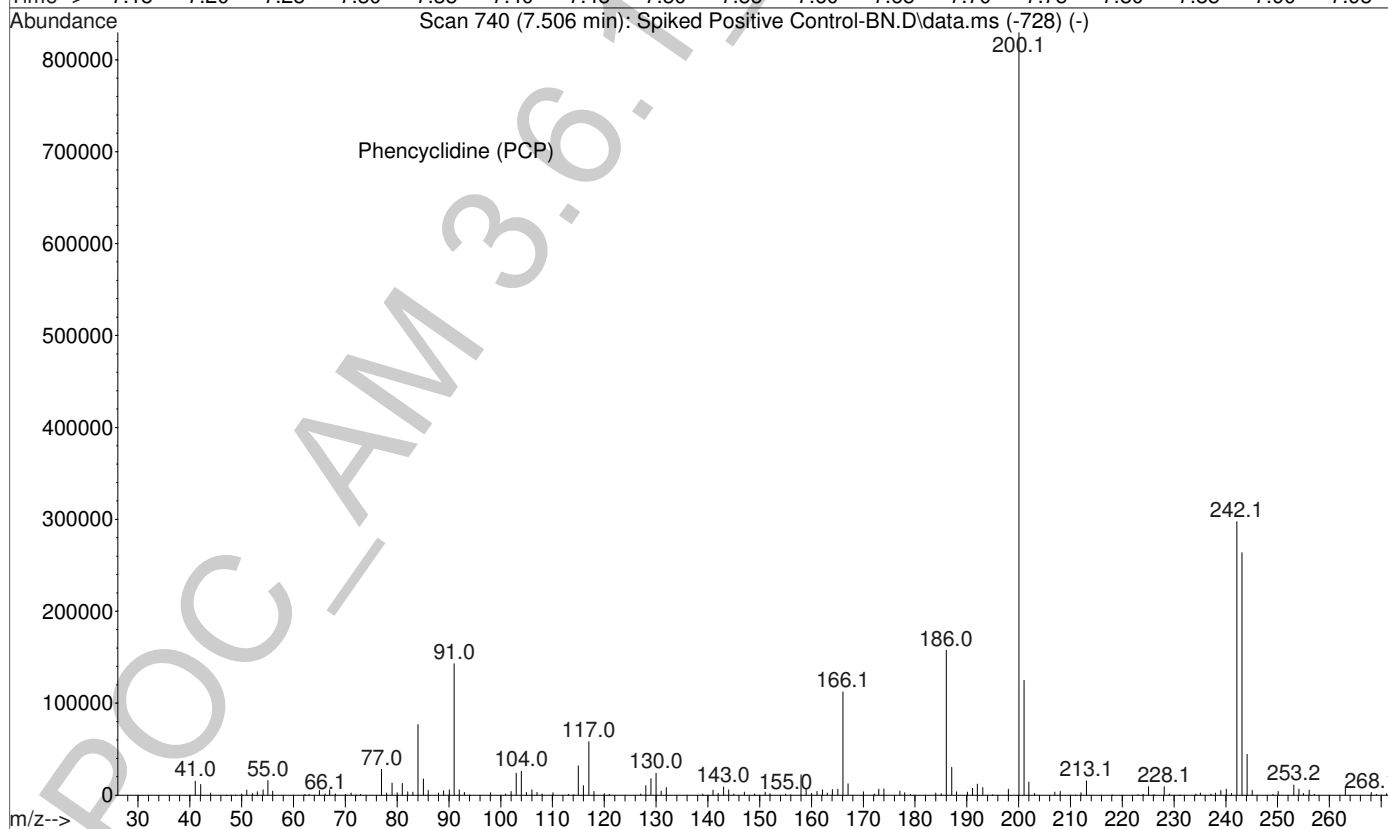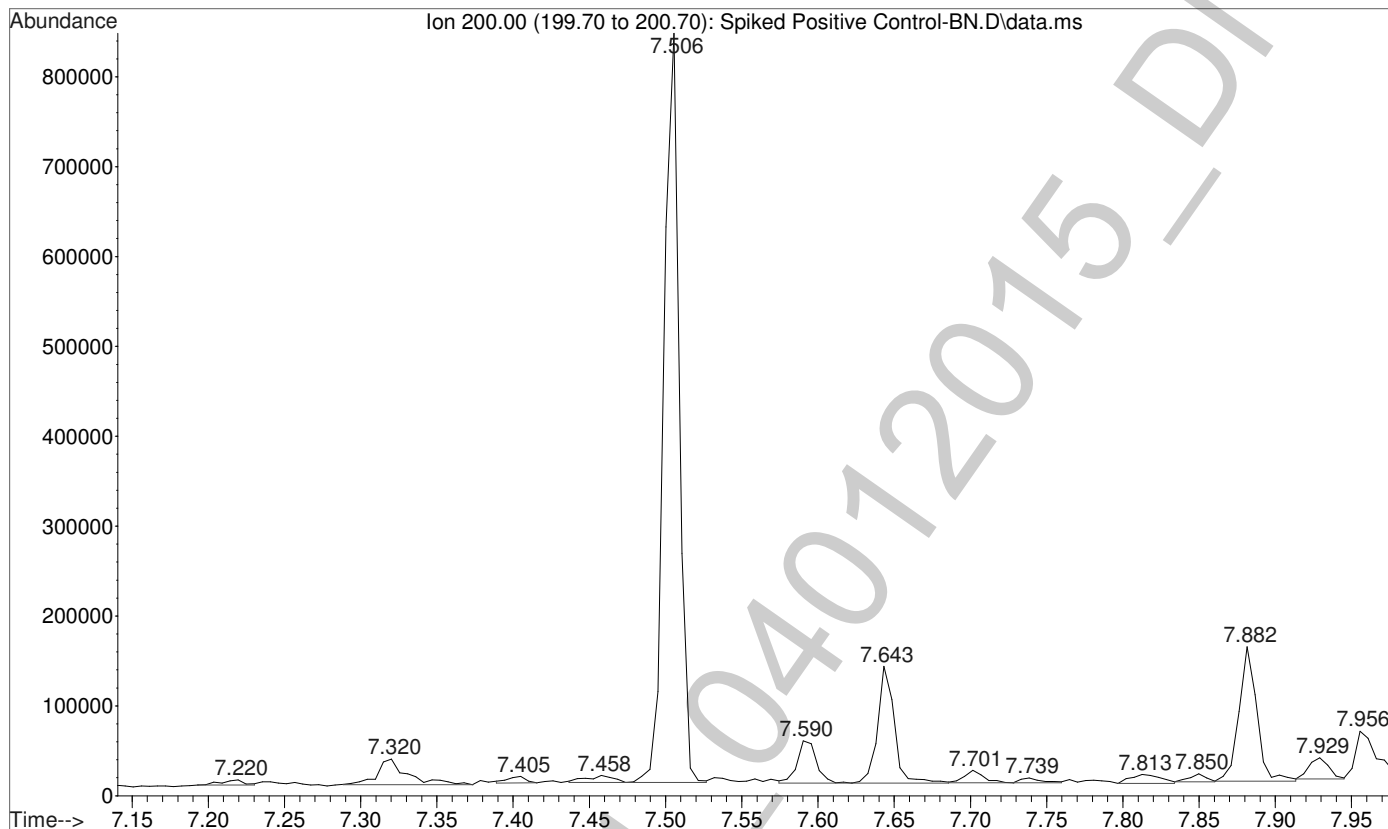



File :C:\gcms\1\data\Blood\040115BN\Spiked Positive Control-BN.D  
Operator : 5LAB-C01\ISPuser  
Acquired : 01 Apr 2015 23:32 using AcqMethod BNSB120510.M  
Instrument : Major Mass Spec  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1  
Vial Number: 2

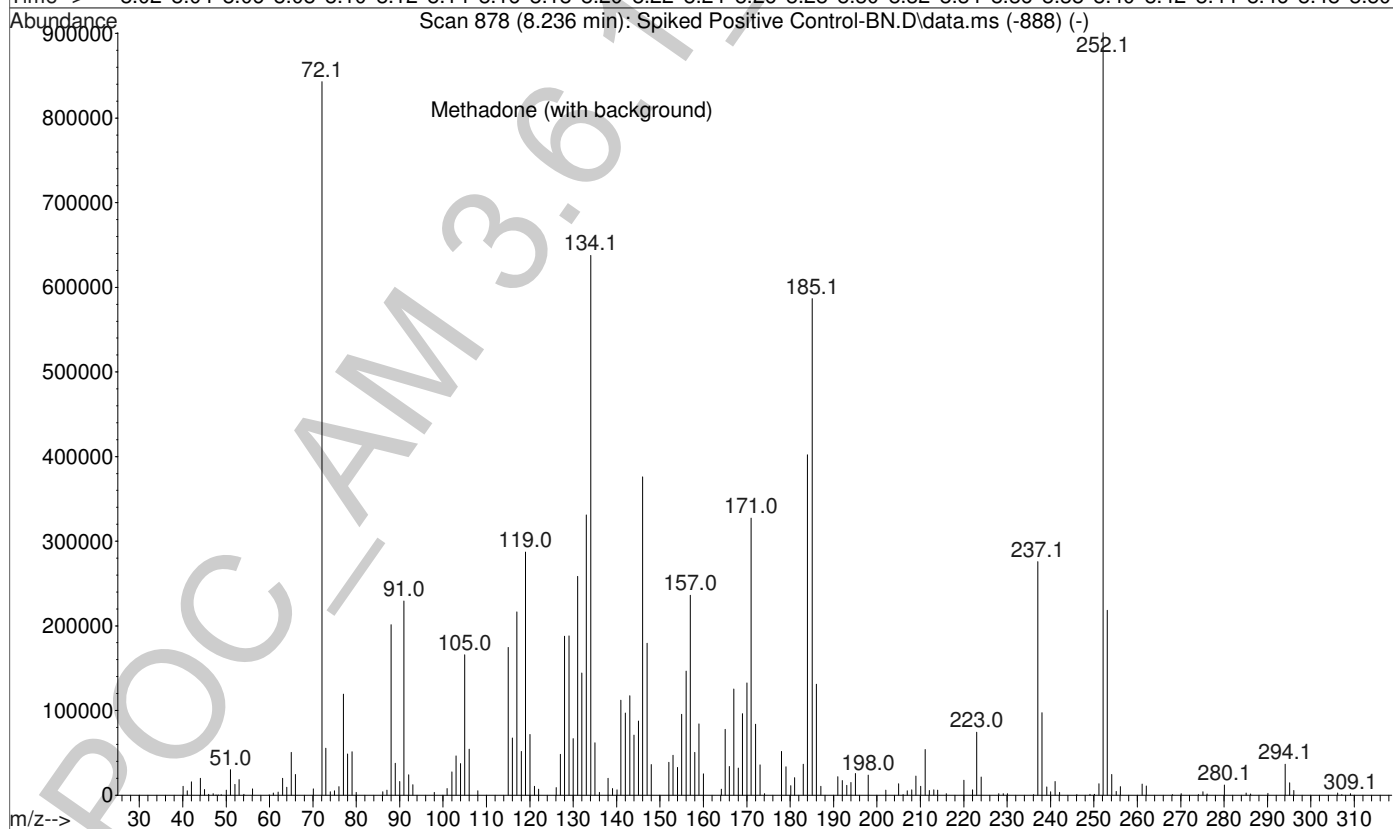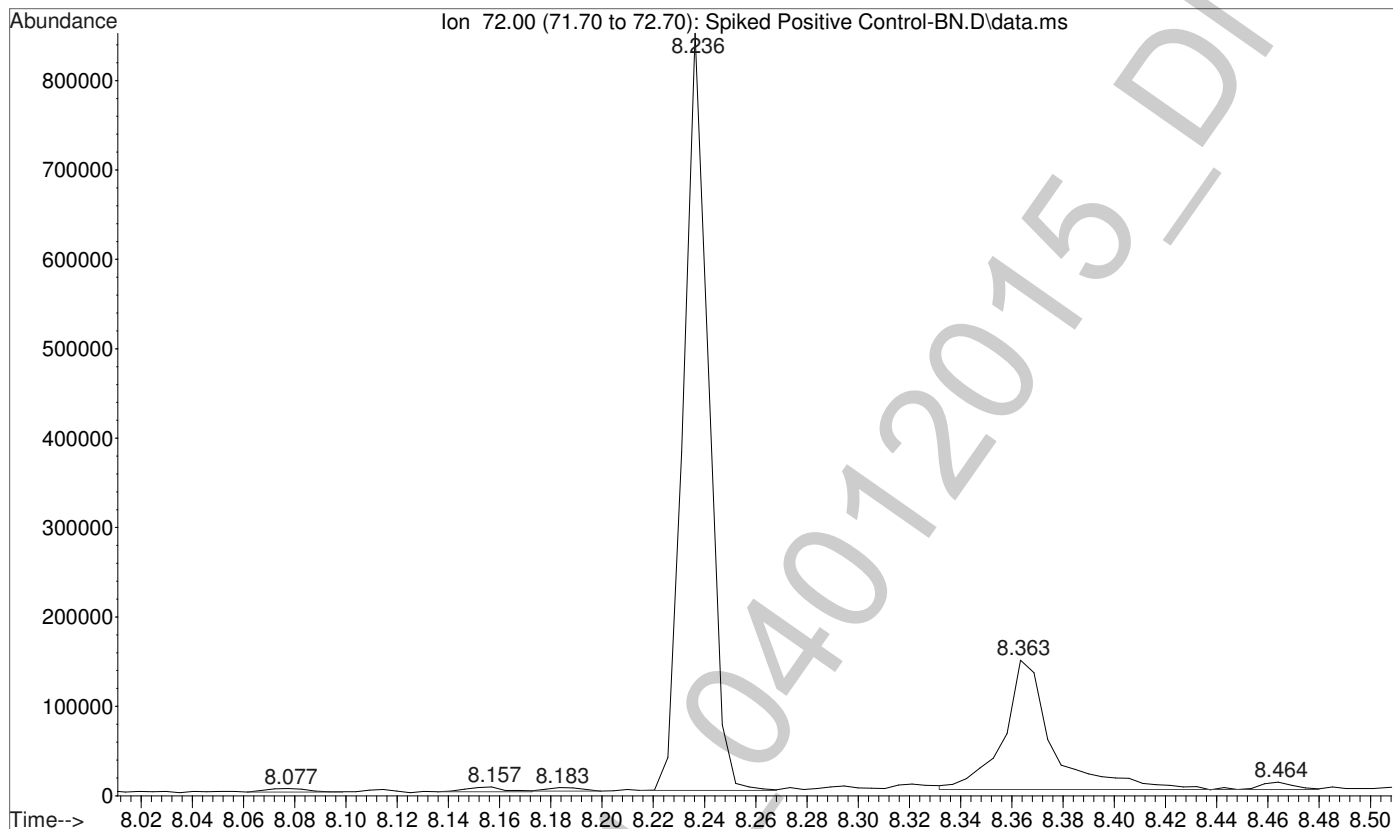

File :C:\gcms\1\data\Blood\040115BN\Spiked Positive Control-BN.D  
Operator : 5LAB-C01\ISPuser  
Acquired : 01 Apr 2015 23:32 using AcqMethod BNSB120510.M  
Instrument : Major Mass Spec  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1  
Vial Number: 2

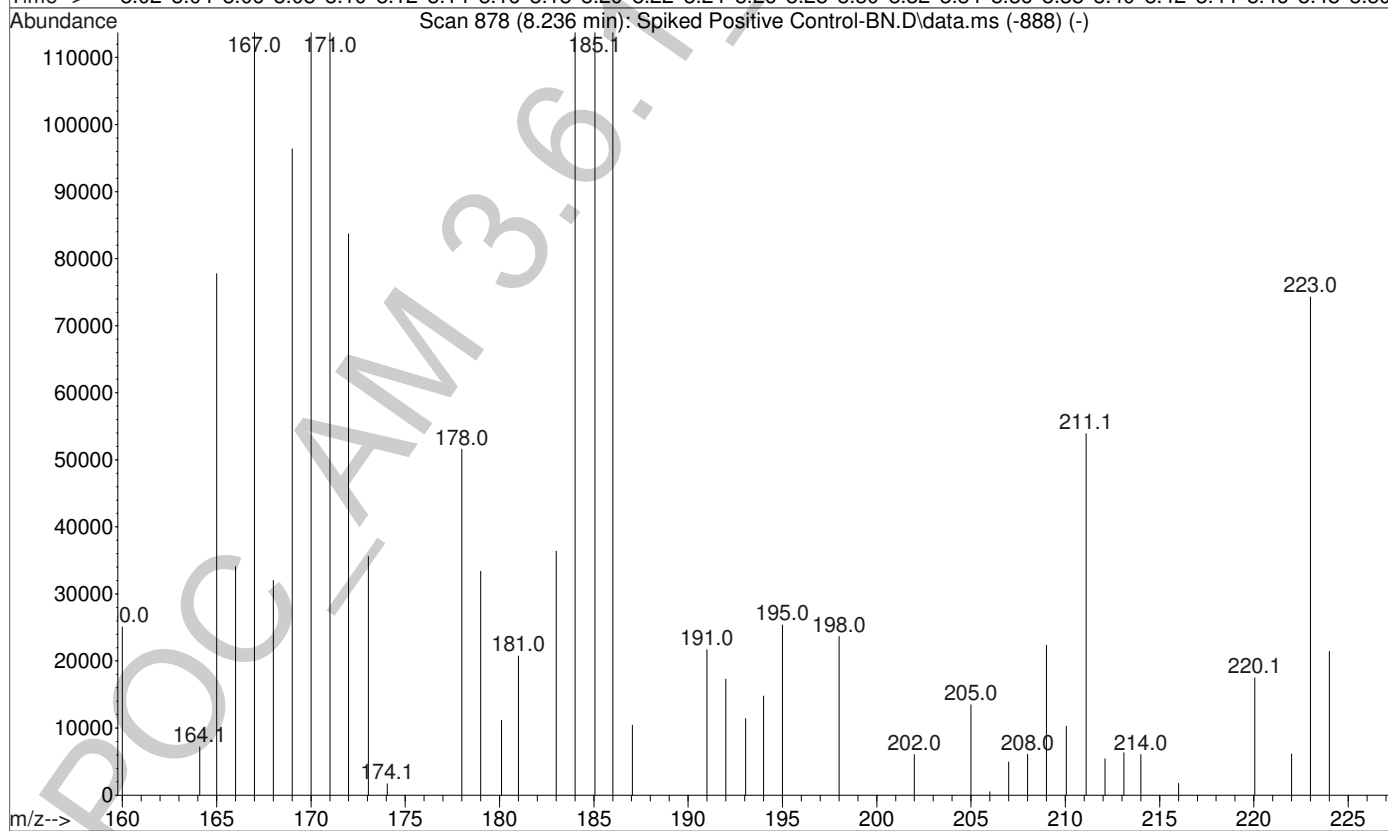
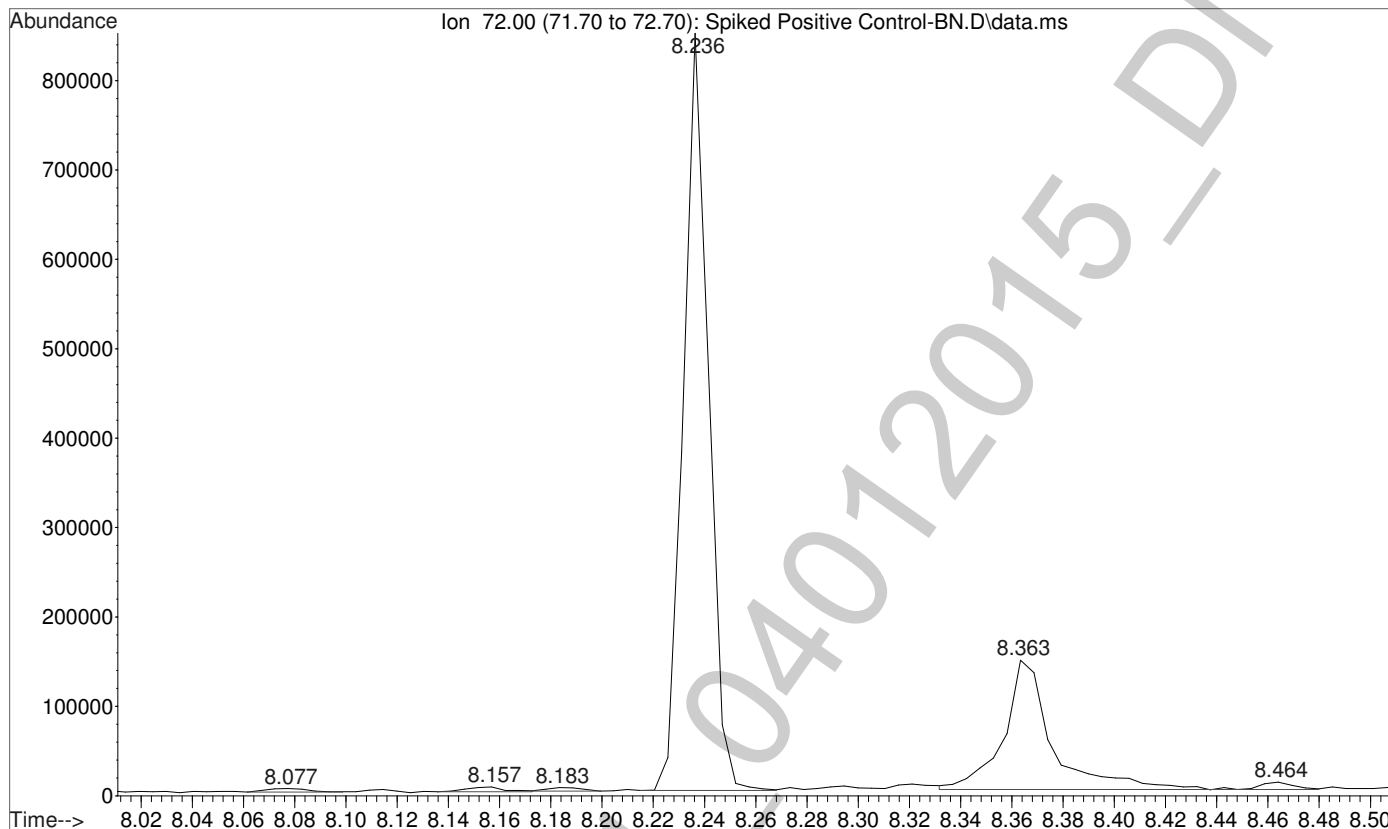


File :C:\gcms\1\data\Blood\040115BN\Spiked Positive Control-BN.D  
Operator : 5LAB-C01\ISPuser  
Acquired : 01 Apr 2015 23:32 using AcqMethod BNSB120510.M  
Instrument : Major Mass Spec  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1  
Vial Number: 2

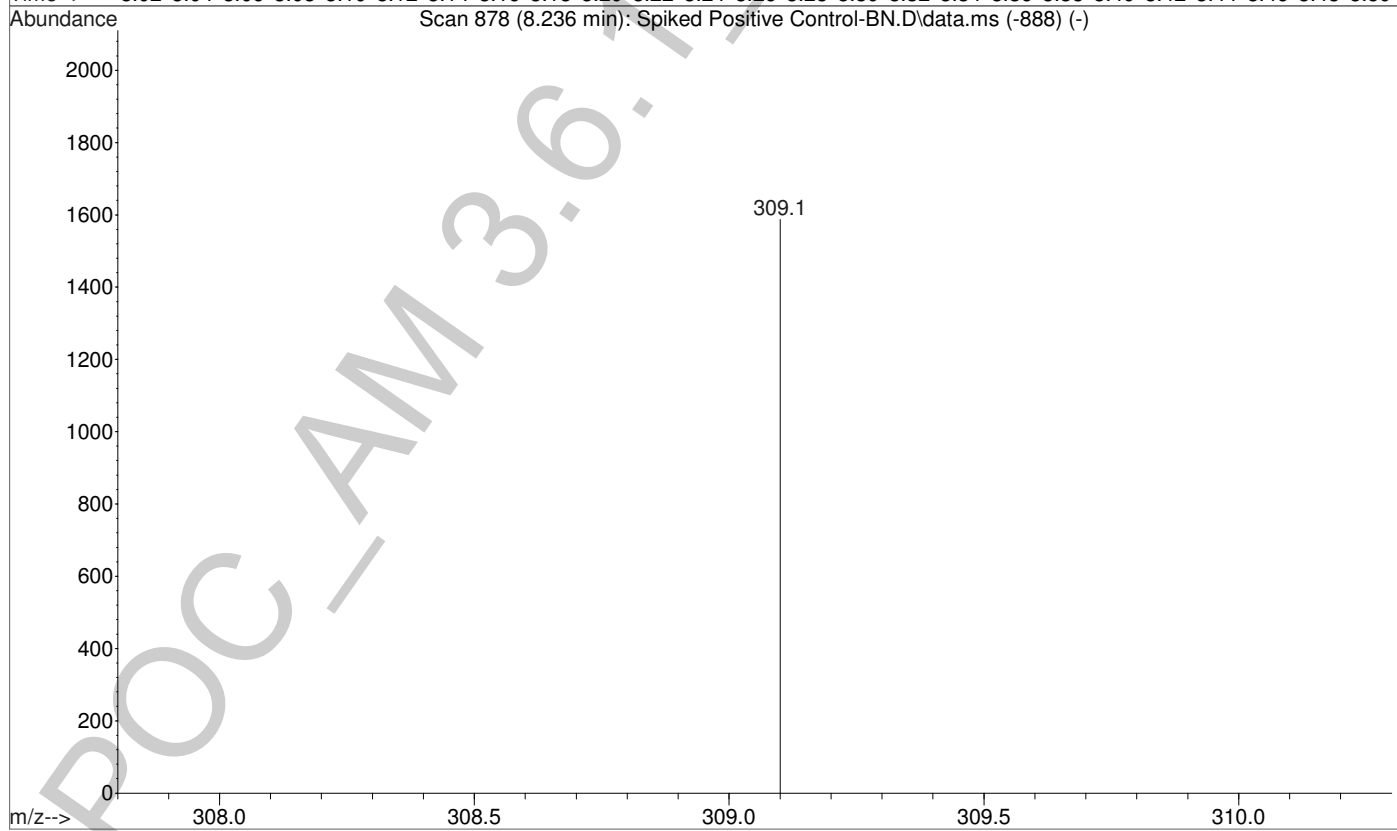
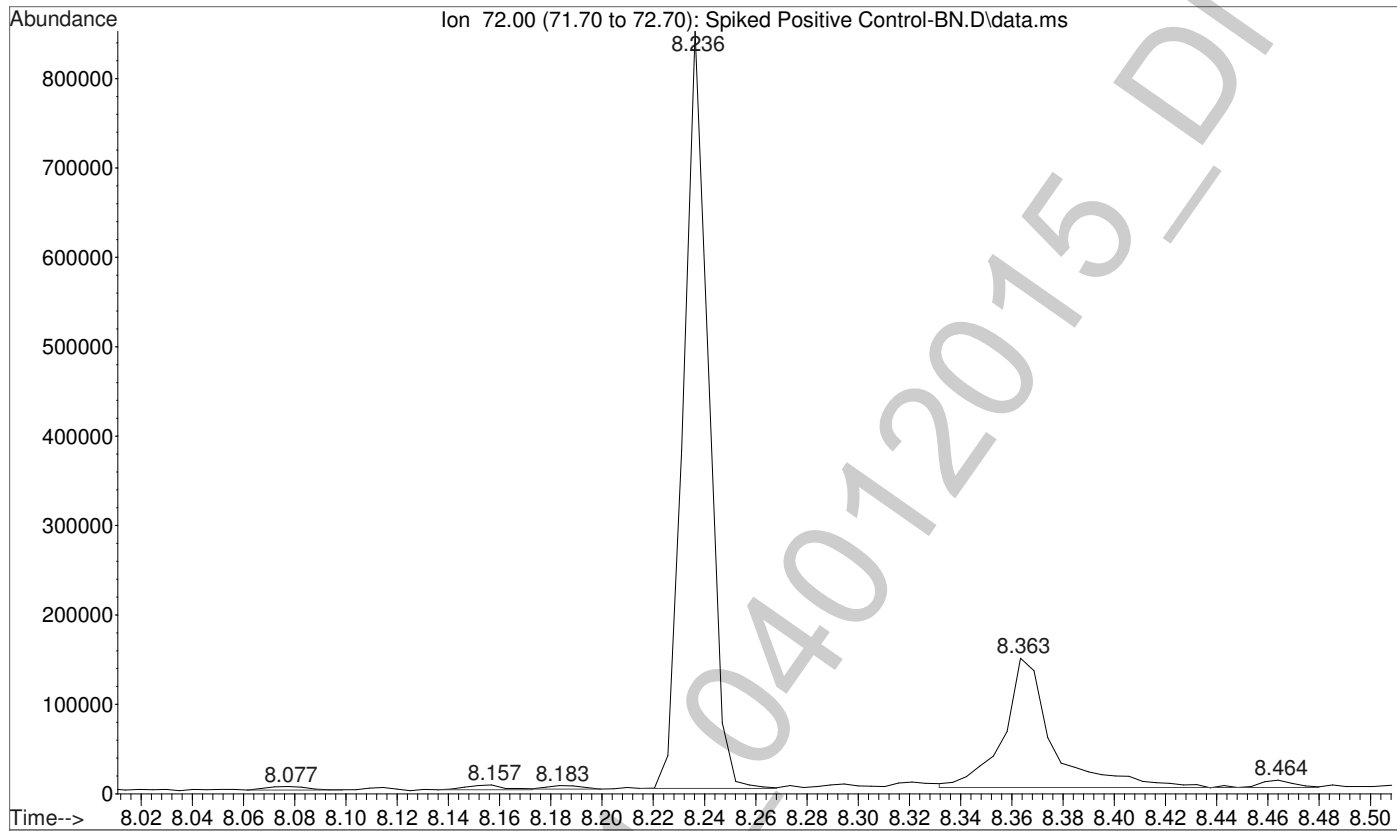






File :C:\gcms\1\data\Blood\040115BN\Spiked Positive Control-BN.D  
Operator : 5LAB-C01\ISPuser  
Acquired : 01 Apr 2015 23:32 using AcqMethod BNSB120510.M  
Instrument : Major Mass Spec  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1  
Vial Number: 2

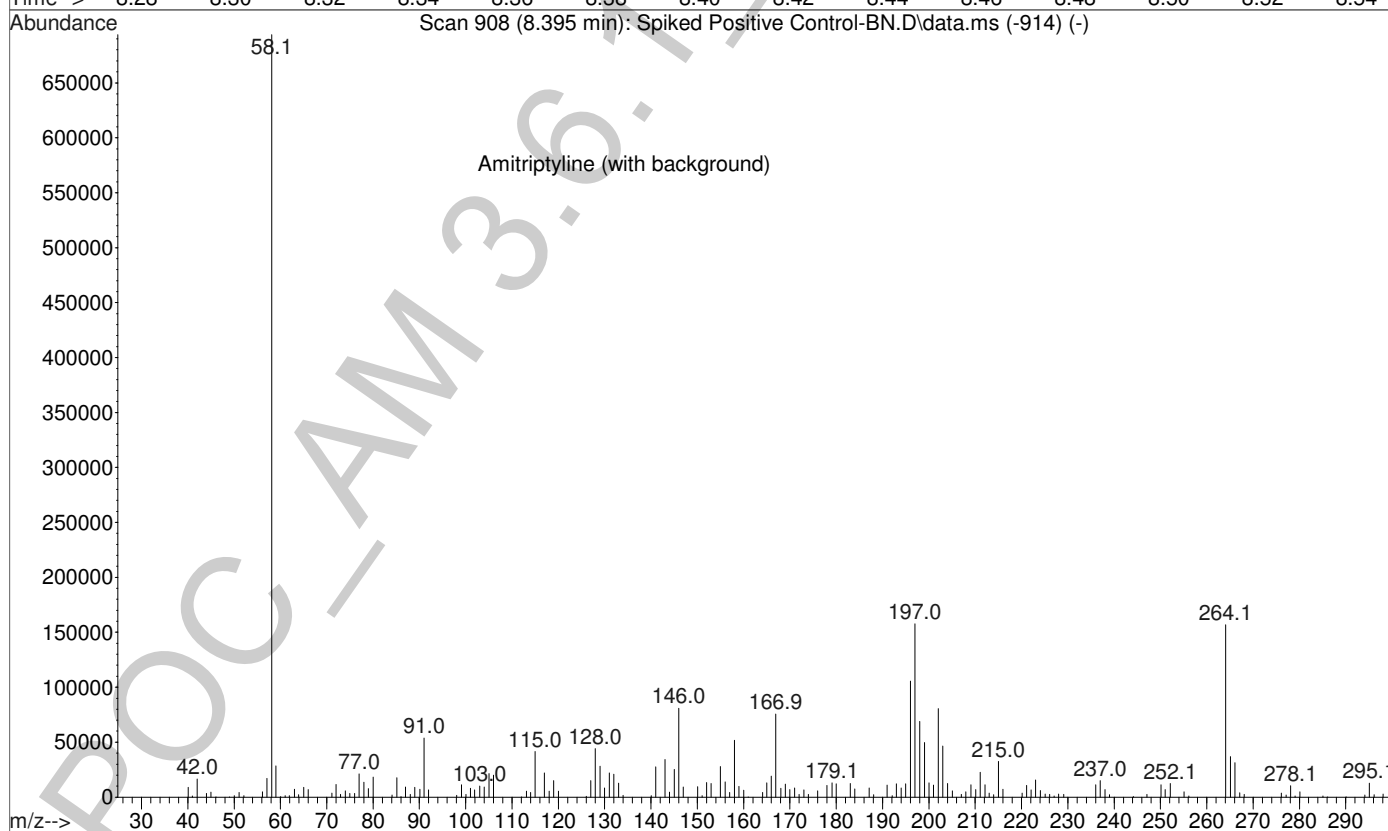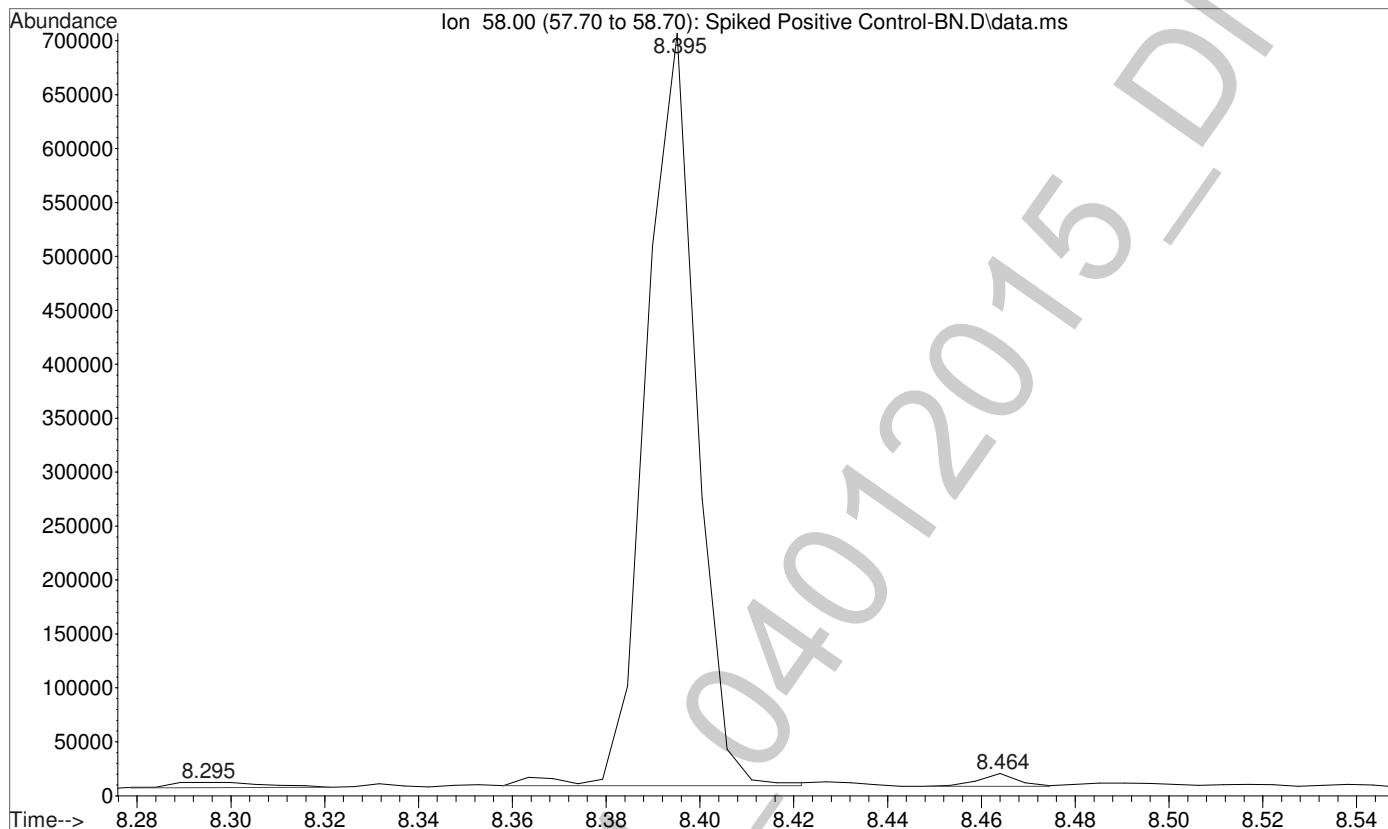



File :C:\gcms\1\data\Blood\040115BN\Spiked Positive Control-BN.D  
Operator : 5LAB-C01\ISPuser  
Acquired : 01 Apr 2015 23:32 using AcqMethod BNSB120510.M  
Instrument : Major Mass Spec  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1  
Vial Number: 2

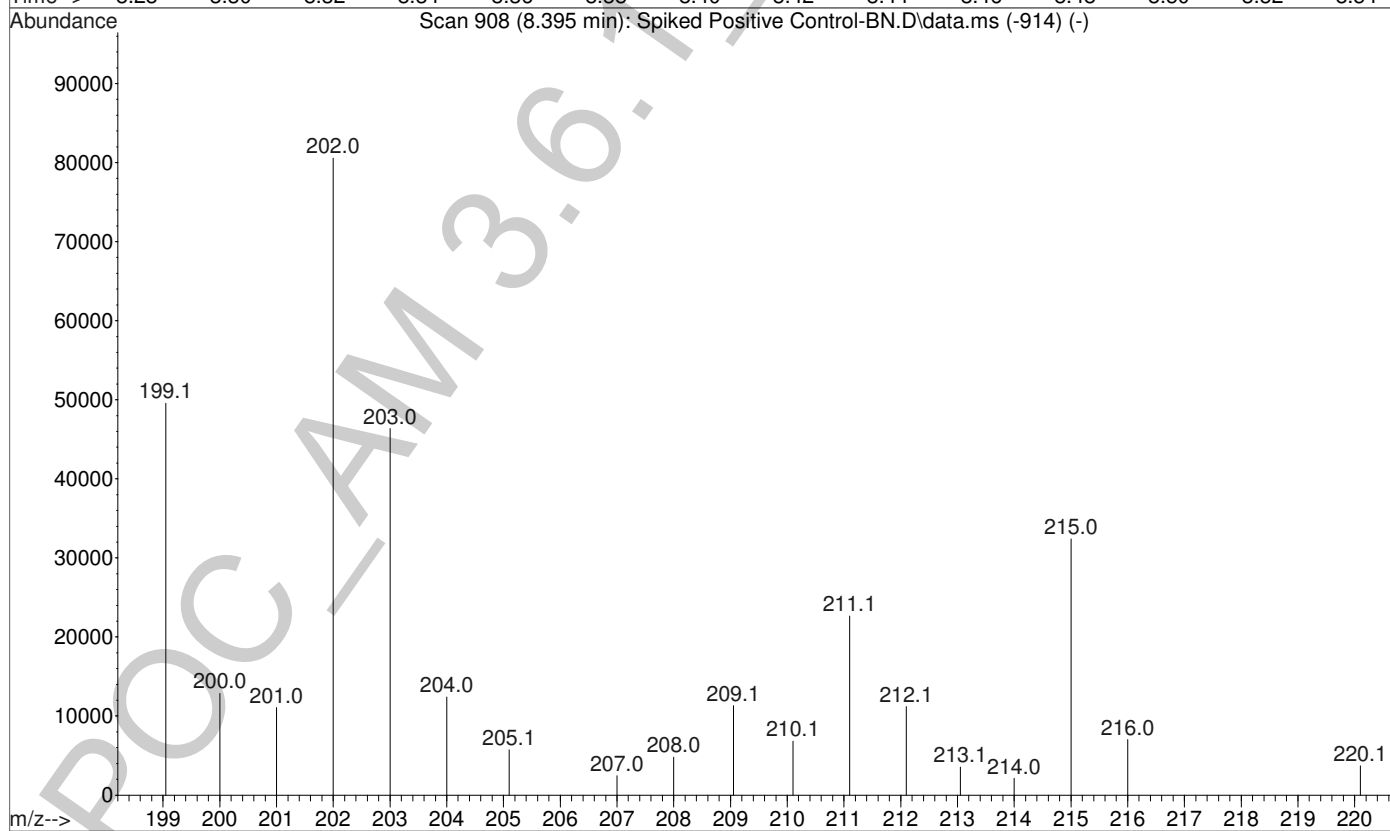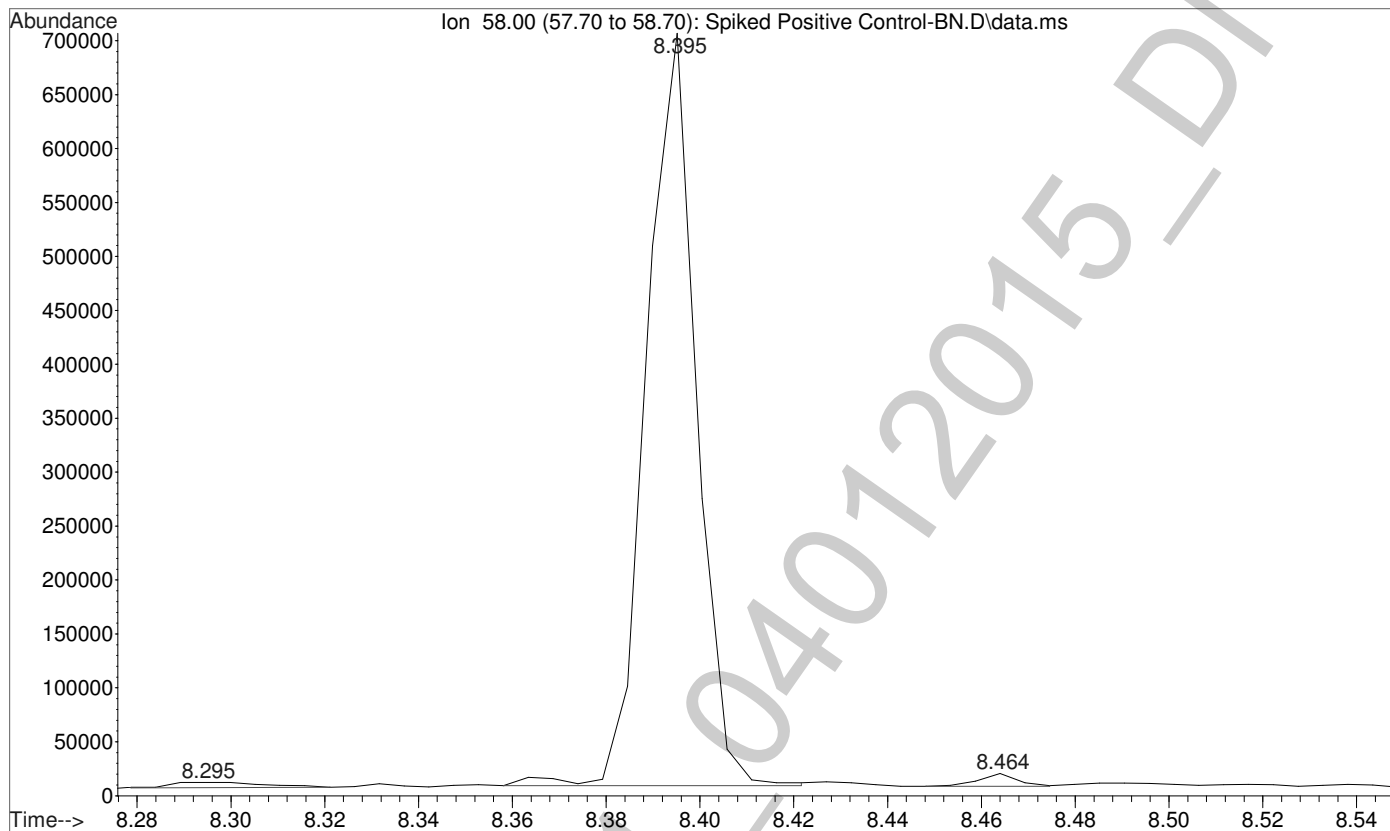



File :C:\gcms\1\data\Blood\040115BN\Spiked Positive Control-BN.D  
Operator : 5LAB-C01\ISPuser  
Acquired : 01 Apr 2015 23:32 using AcqMethod BNSB120510.M  
Instrument : Major Mass Spec  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1  
Vial Number: 2

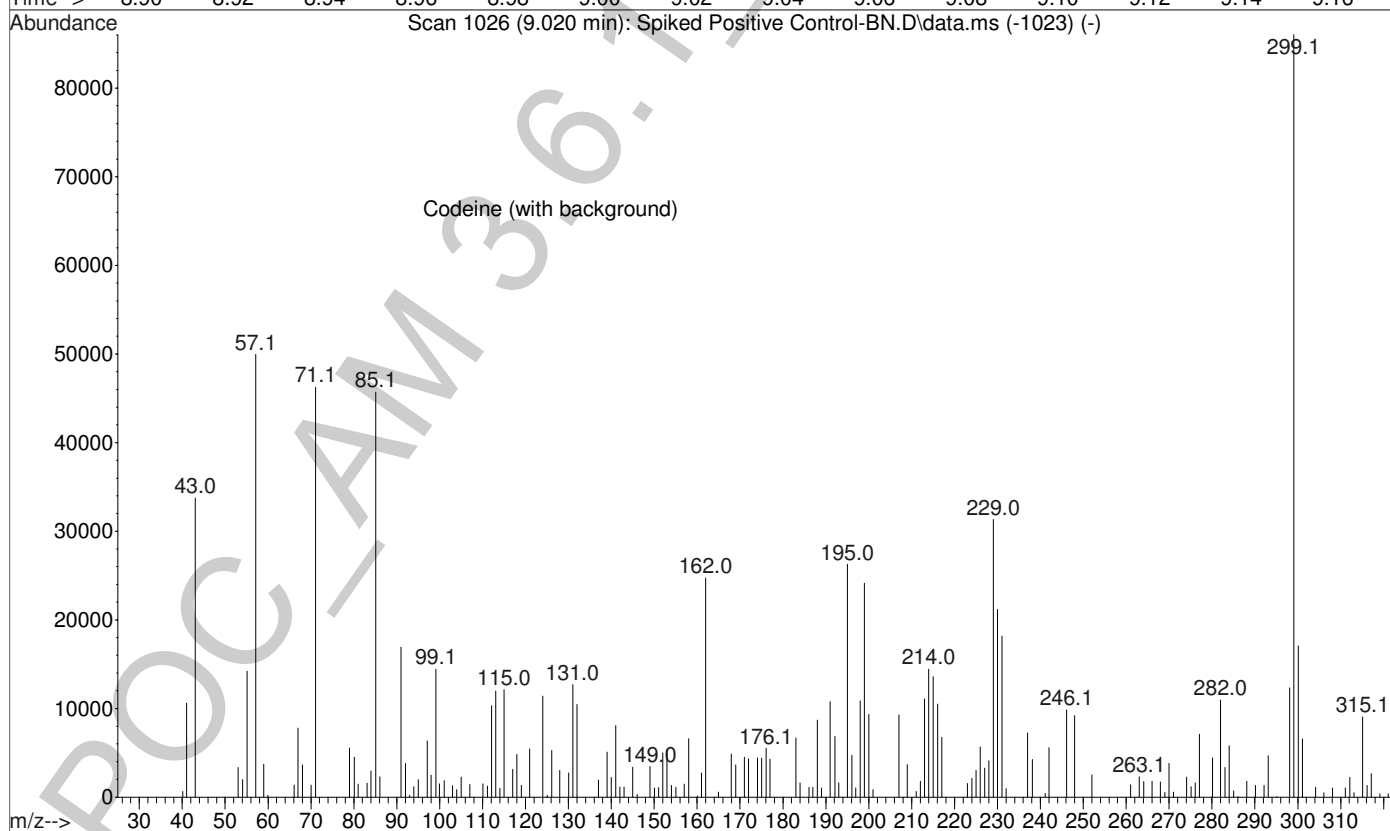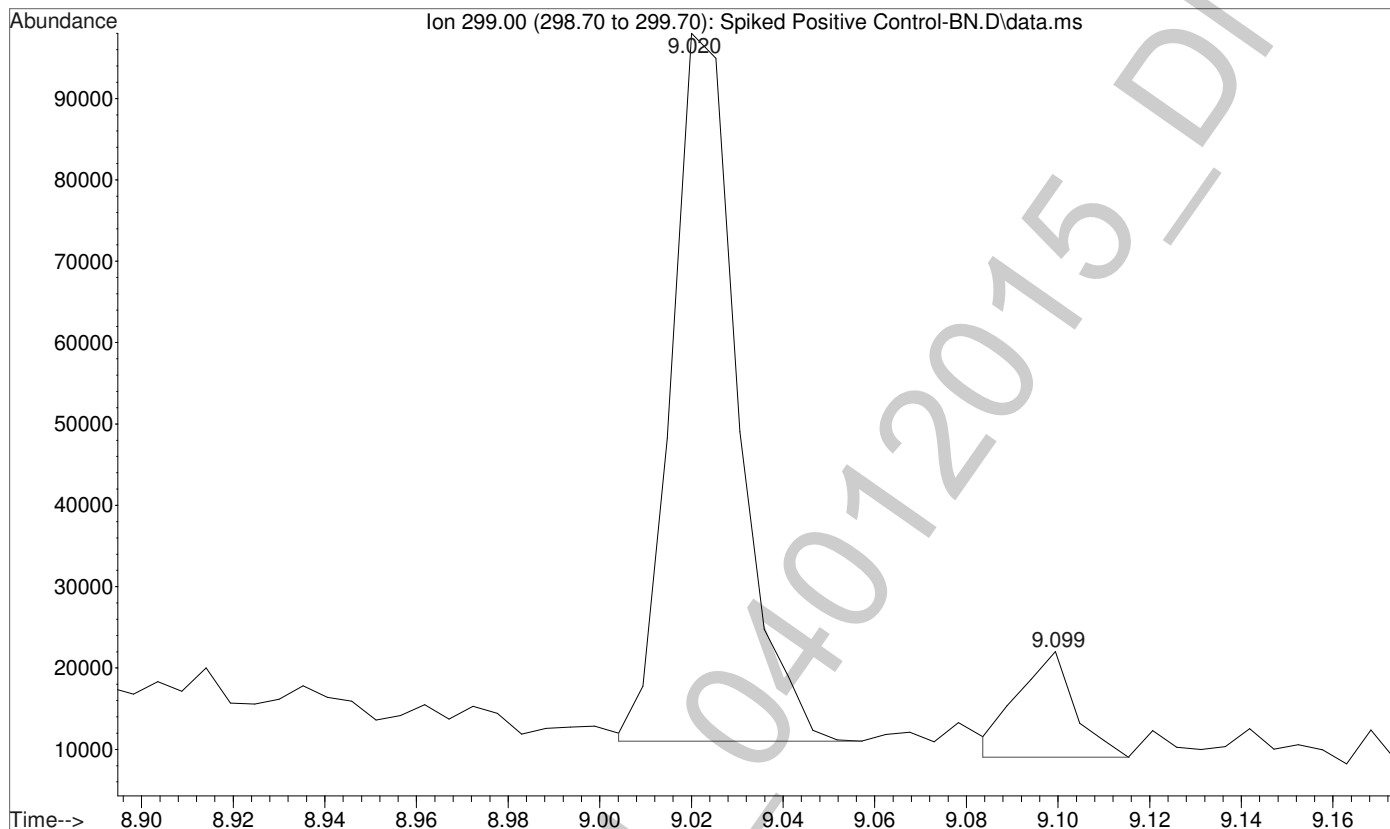

File :C:\gcms\1\data\Blood\040115BN\Spiked Positive Control-BN.D  
Operator : 5LAB-C01\ISPuser  
Acquired : 01 Apr 2015 23:32 using AcqMethod BNSB120510.M  
Instrument : Major Mass Spec  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1  
Vial Number: 2

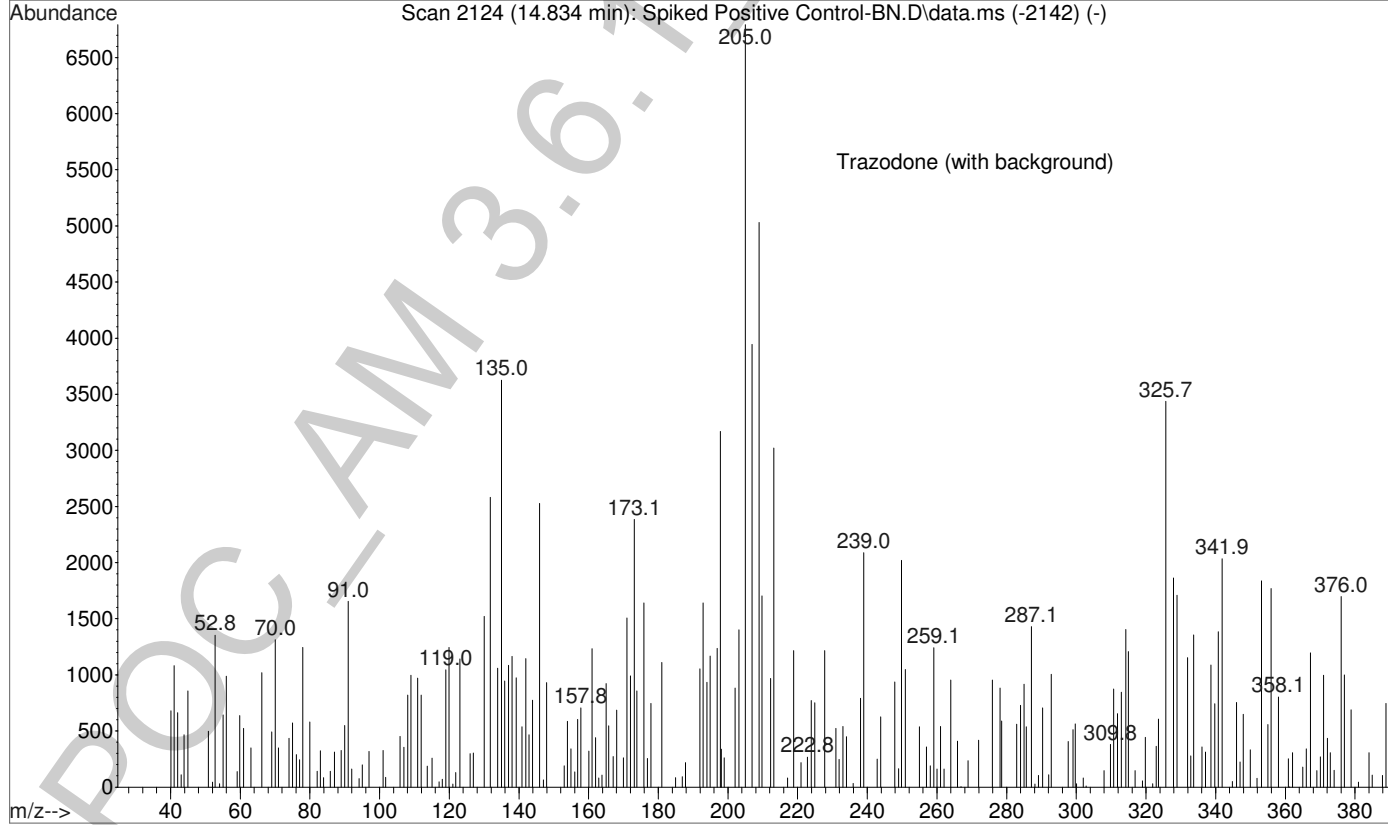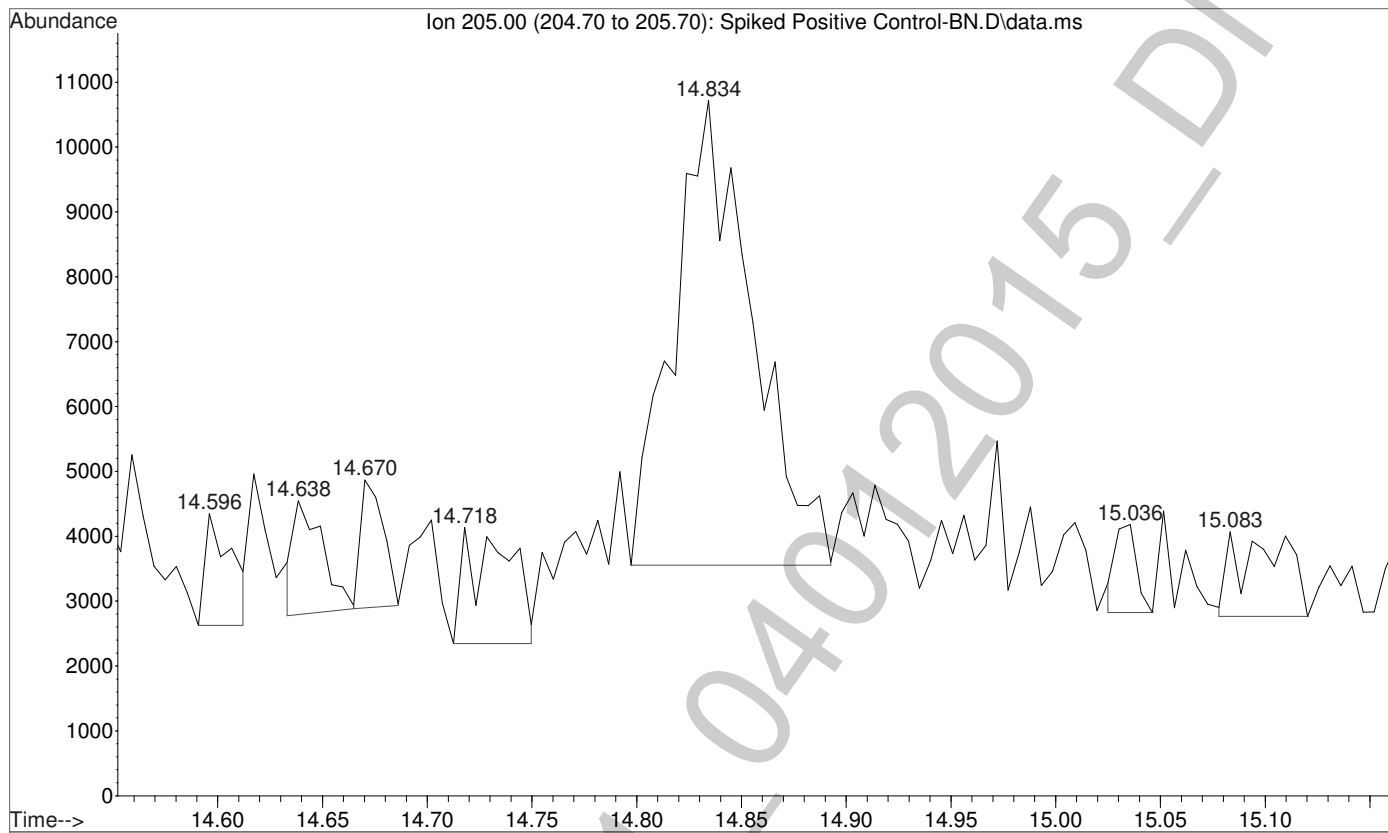

File :C:\gcms\1\data\Blood\040115BN\prbLK2.D  
Operator : 5LAB-C01\ISPuser  
Acquired : 01 Apr 2015 23:56 using AcqMethod BNSB120510.M  
Instrument : Major Mass Spec  
Sample Name: Solvent Blank  
Misc Info : Chloroform  
Vial Number: 99

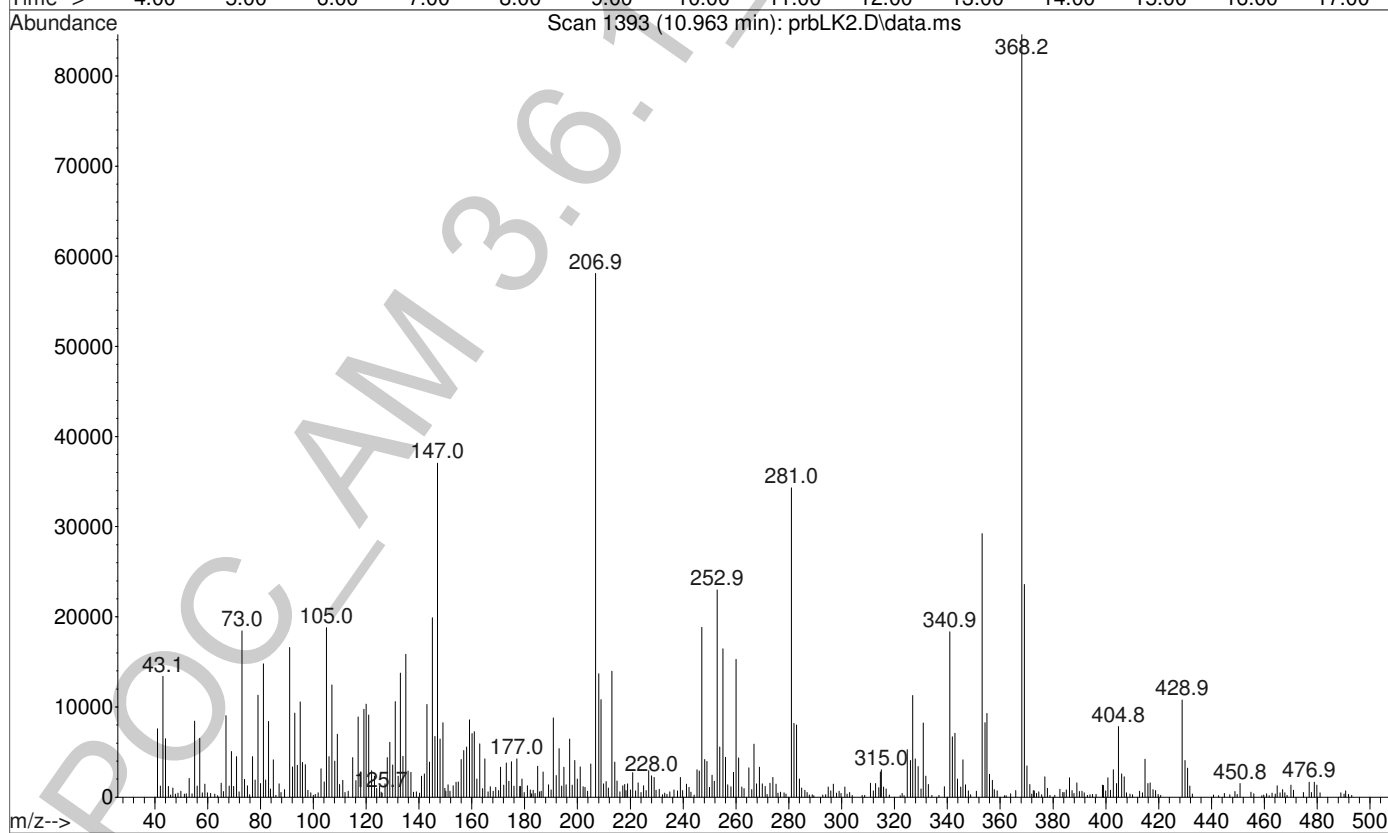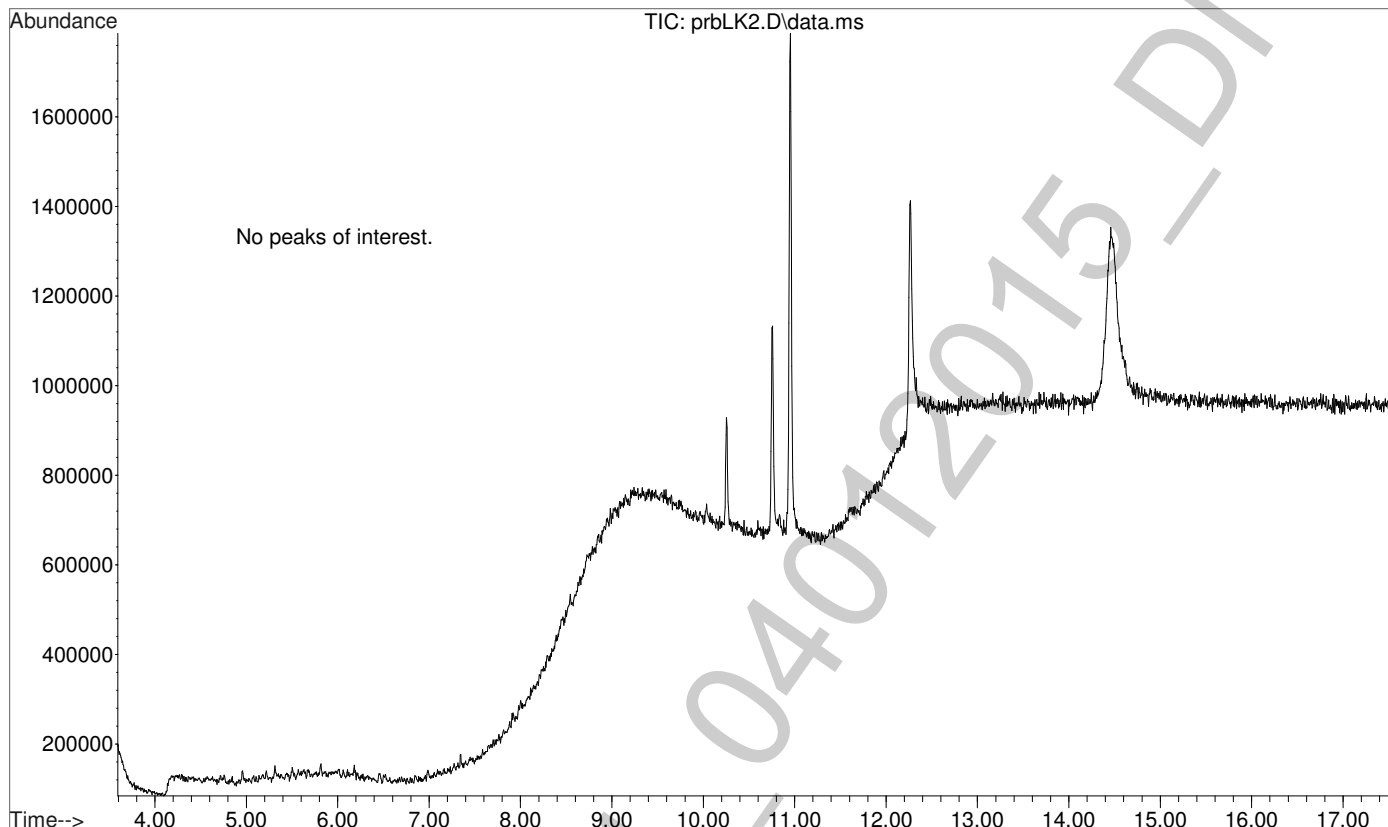

Analytical Method 3.6.1 & 3.6.7 QA Check List

Run Start Date: 04/01/15

Analyst: DND

(Long GC/MS temperature program)

Positive Control Compound List

- Methamphetamine
- Nicotine
- Meperidine
- Caffeine
- Diphenhydramine
- Lidocaine
- PCP
- Methadone
- Amitriptyline
- Codeine
- (Trazodone)



Internal Standards

- Benzphetamine
- Papaverine


Optional back extraction **not** performed.  
Samples reconstituted in methanol.



File :C:\gcms\1\data\Blood\040115BN\Reinjection Longer GC Method\P  
... rerun Solvent Blankr.D  
Operator : 5LAB-C01\ISPuser  
Instrument : Major Mass Spec  
Acquired : 02 Apr 2015 00:18 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Pre-run Solvent Blank  
Misc Info : Chloroform

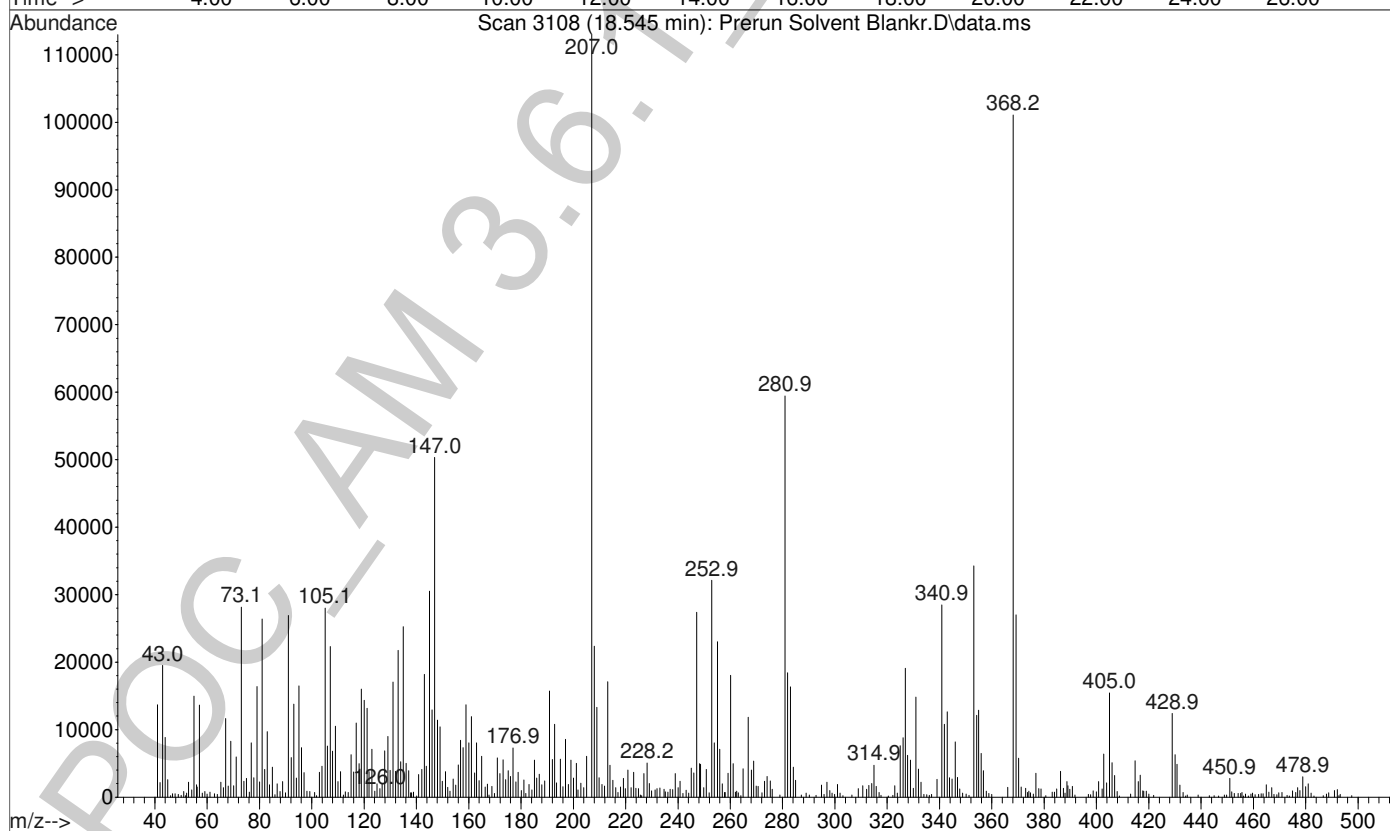
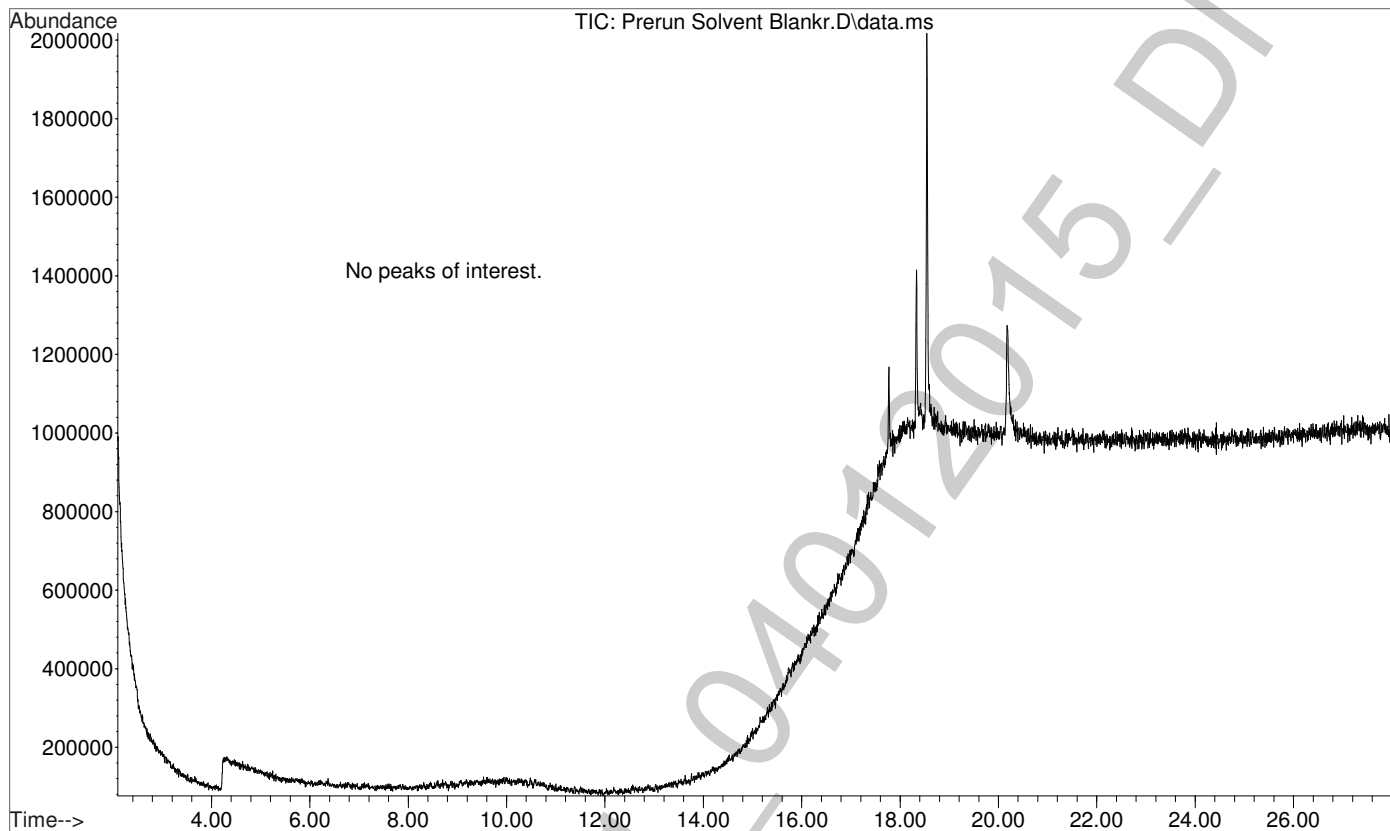


File :C:\gcms\1\data\Blood\040115BN\Reinjection Longer GC Method\N  
... egative Control-BNr.D  
Operator : 5LAB-C01\ISPuser  
Instrument : Major Mass Spec  
Acquired : 02 Apr 2015 00:52 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Negative Control - Utak Lot B0130  
Misc Info : Analytical Method 3.6.1


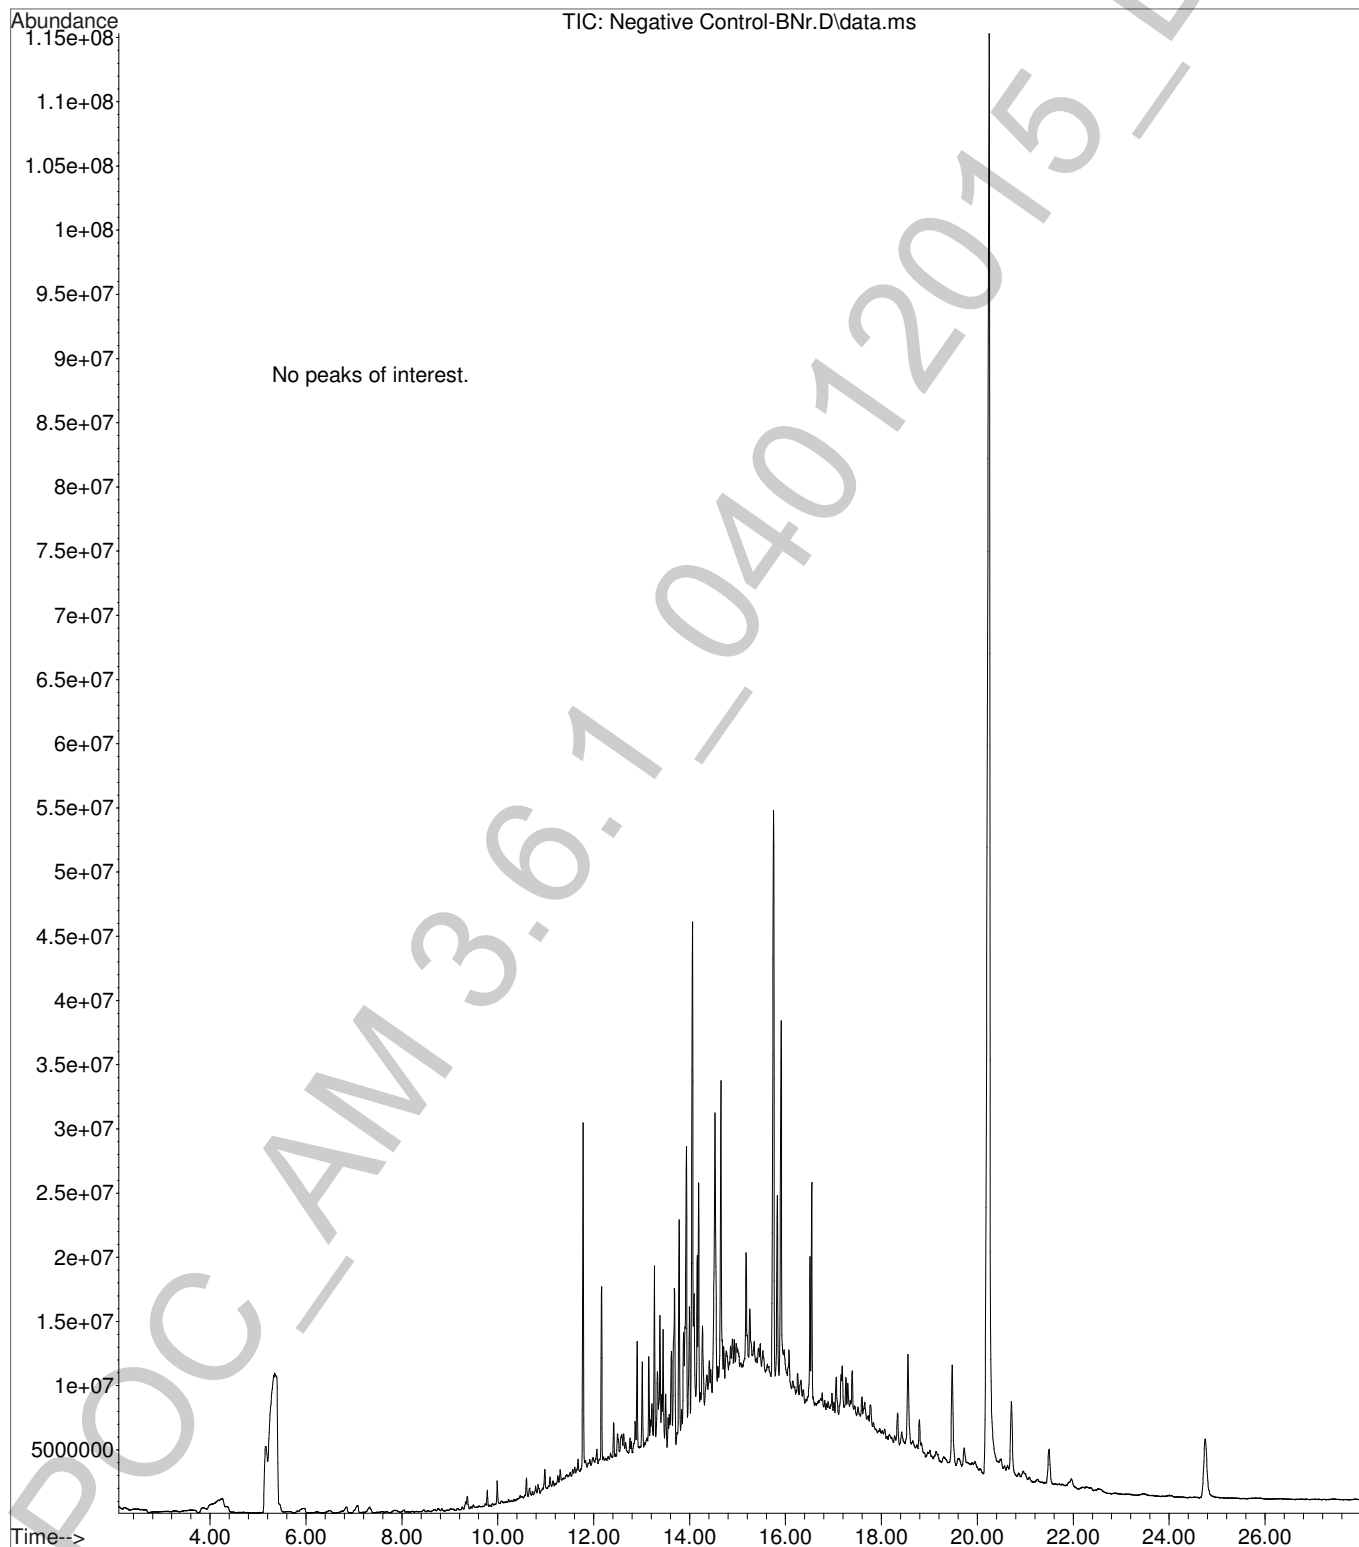





File :C:\gcms\1\data\Blood\040115BN\Reinjection Longer GC Method\N  
... egative Control-BNr.D  
Operator : 5LAB-C01\ISPuser  
Instrument : Major Mass Spec  
Acquired : 02 Apr 2015 00:52 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Negative Control - Utak Lot B0130  
Misc Info : Analytical Method 3.6.1

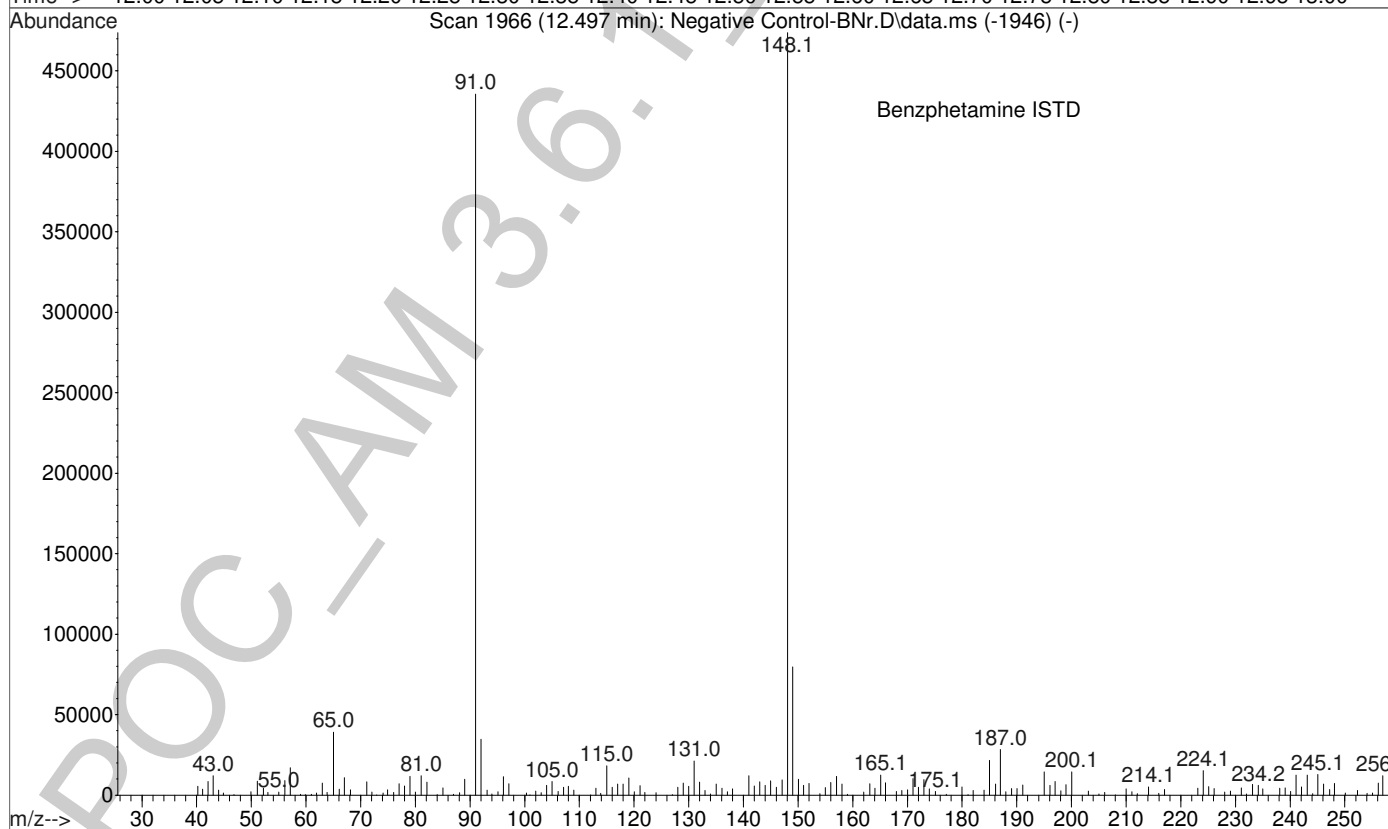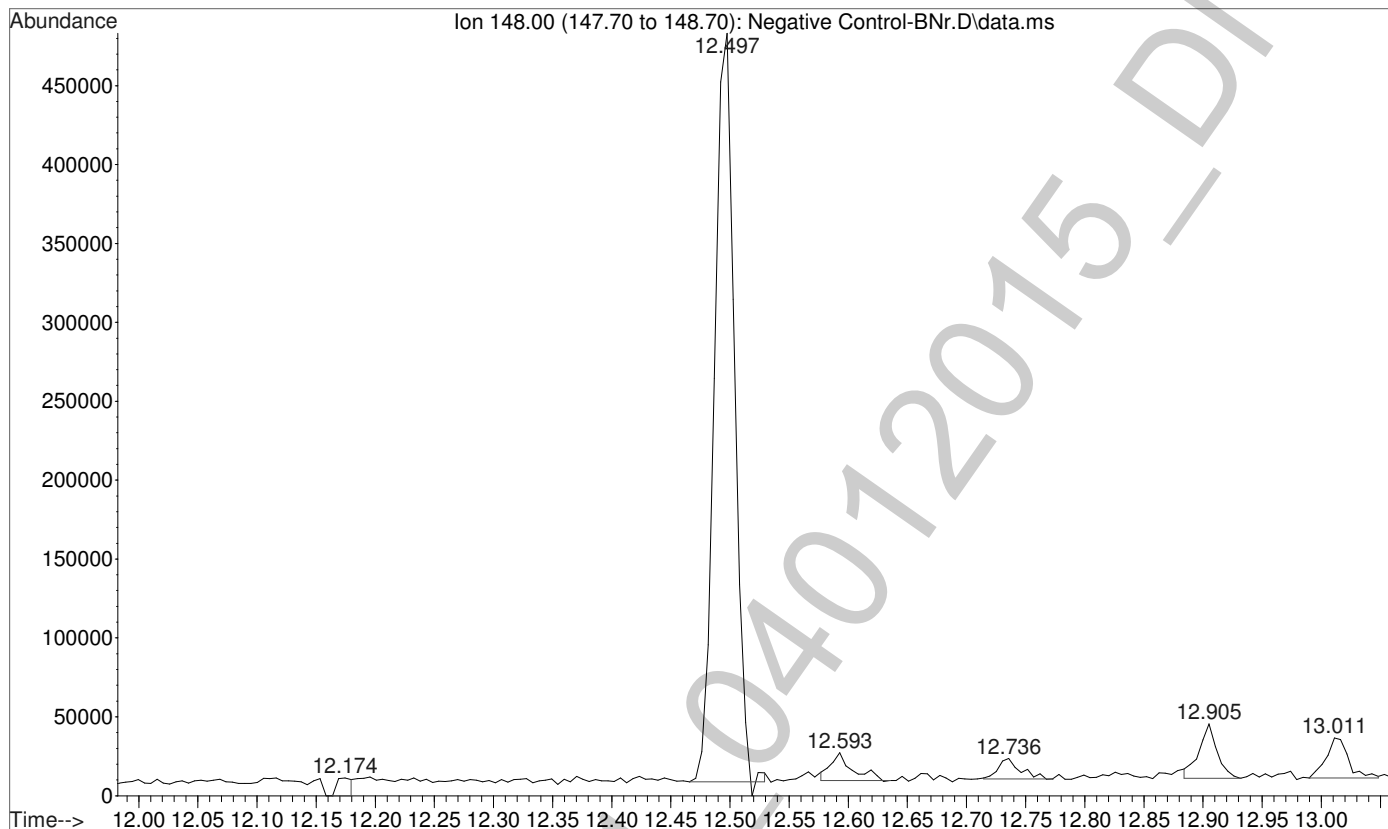



File :C:\gcms\1\data\Blood\040115BN\Reinjection Longer GC Method\N  
... egative Control-BNr.D  
Operator : 5LAB-C01\ISPuser  
Instrument : Major Mass Spec  
Acquired : 02 Apr 2015 00:52 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Negative Control - Utak Lot B0130  
Misc Info : Analytical Method 3.6.1

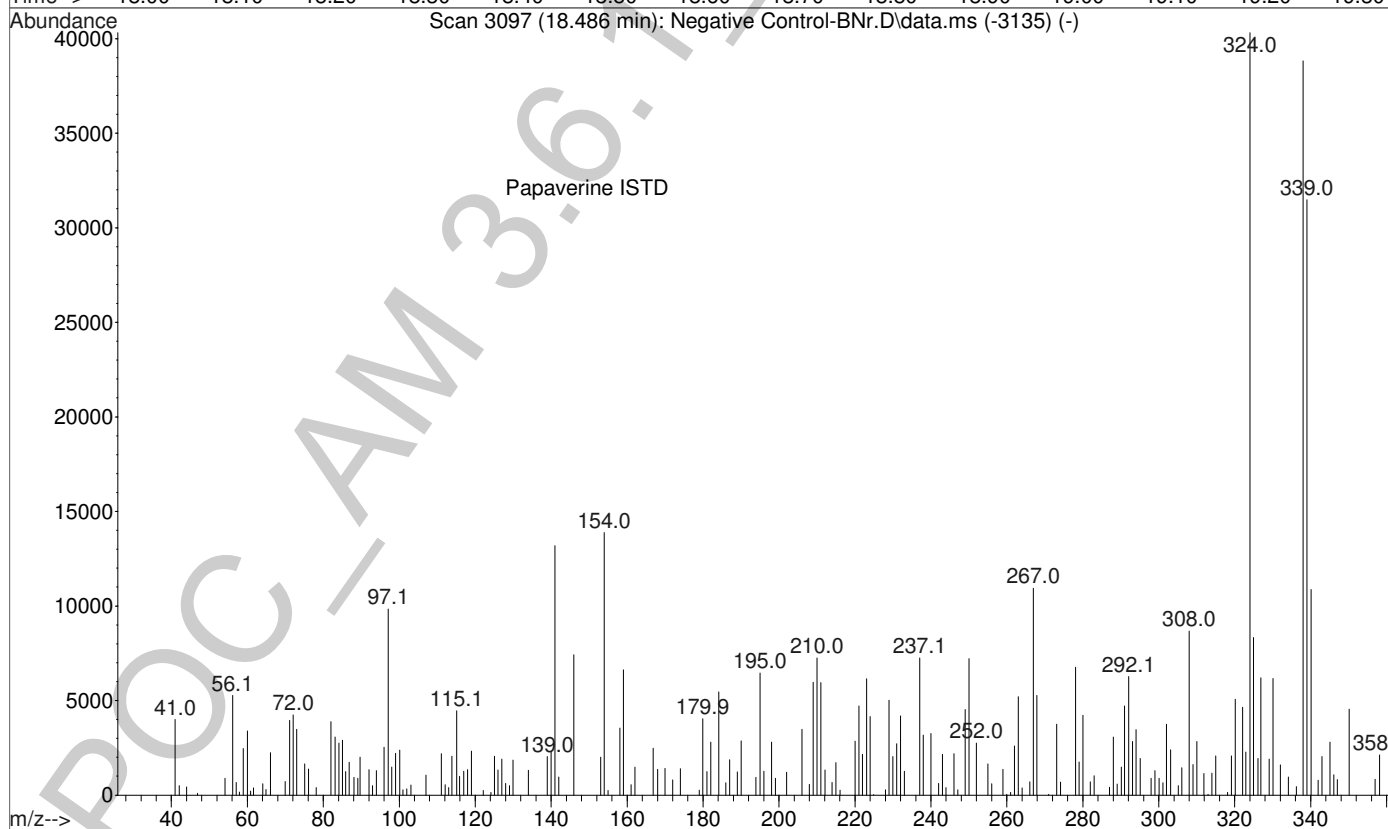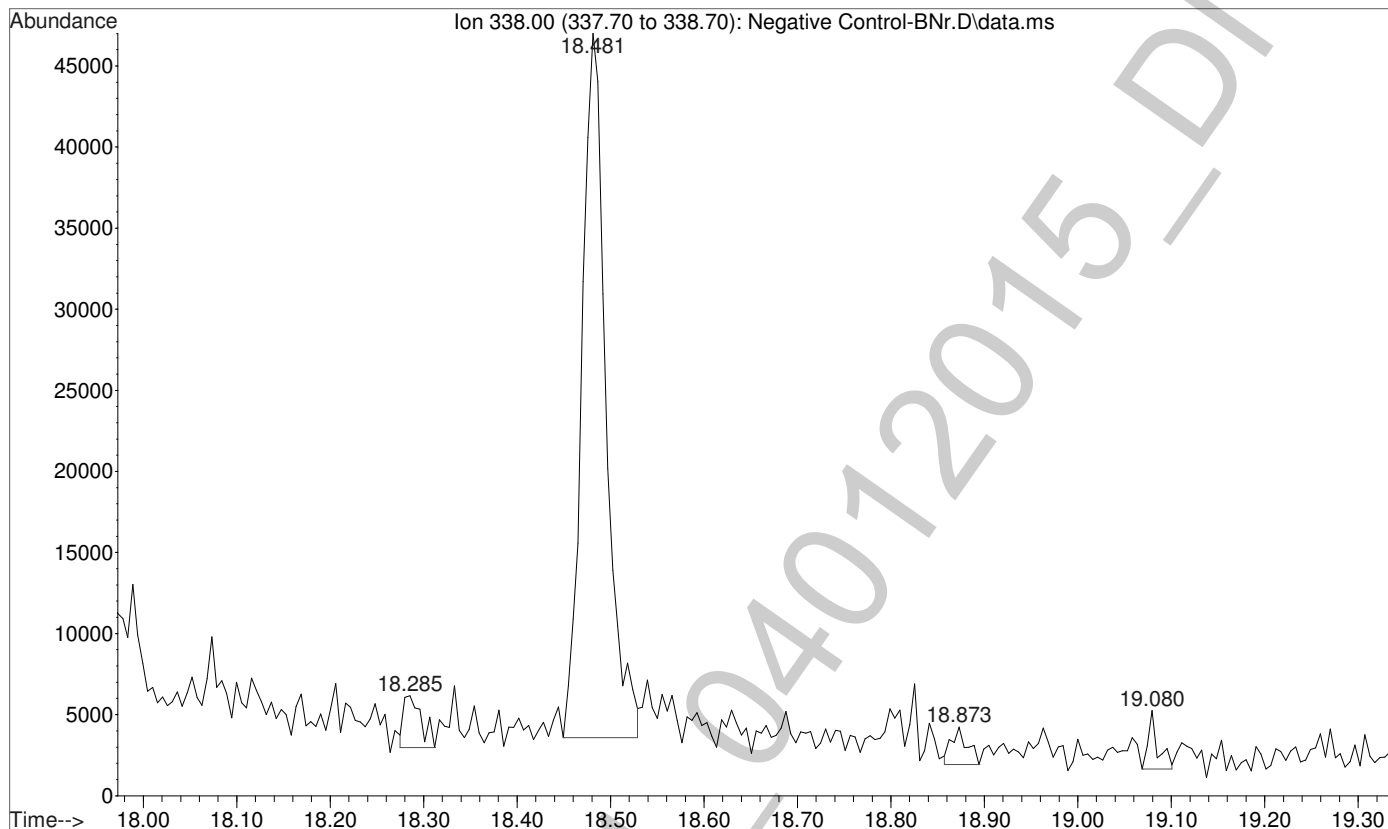



File :C:\gcms\1\data\Blood\040115BN\Reinjection Longer GC Method\S  
... piked Positive Control-BNr.D  
Operator : 5LAB-C01\ISPuser  
Instrument : Major Mass Spec  
Acquired : 02 Apr 2015 01:26 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1

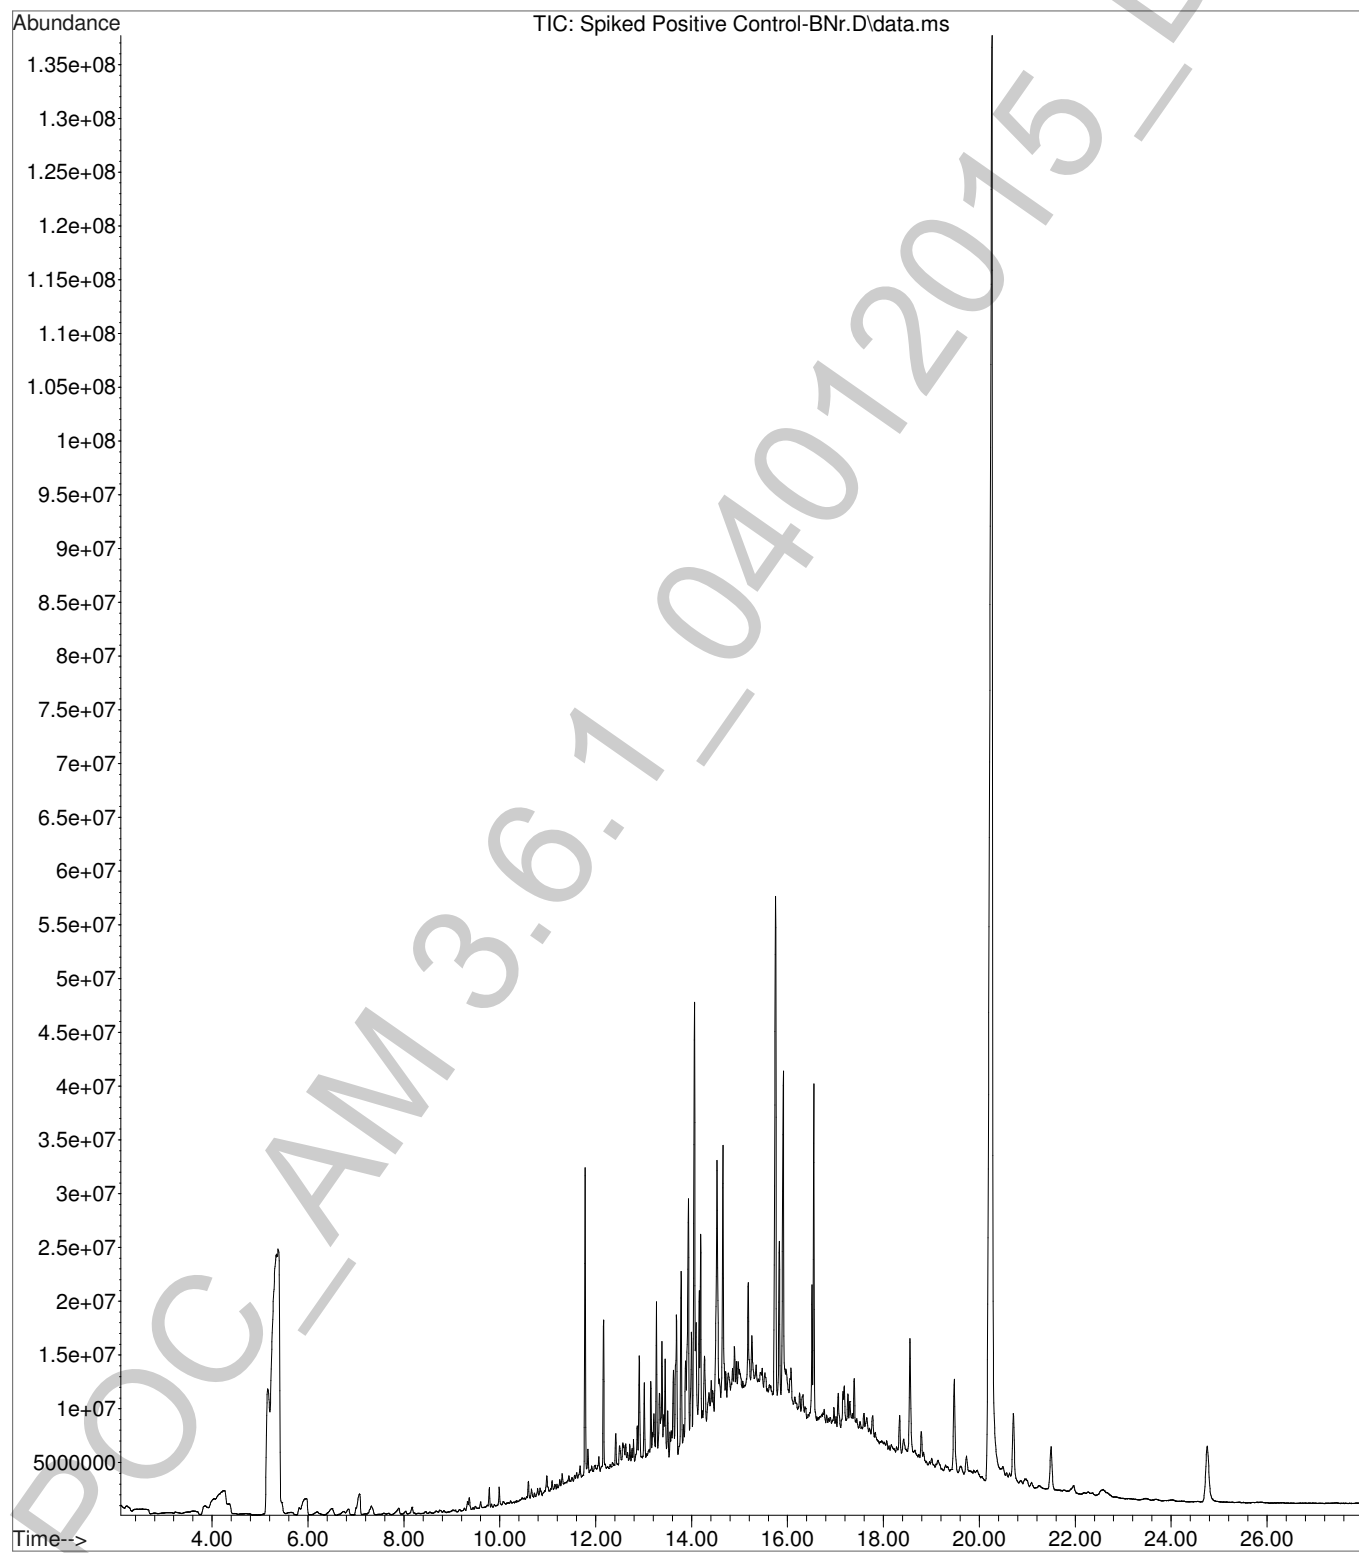



File :C:\gcms\1\data\Blood\040115BN\Reinjection Longer GC Method\S  
... piked Positive Control-BNr.D  
Operator : 5LAB-C01\ISPuser  
Instrument : Major Mass Spec  
Acquired : 02 Apr 2015 01:26 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1

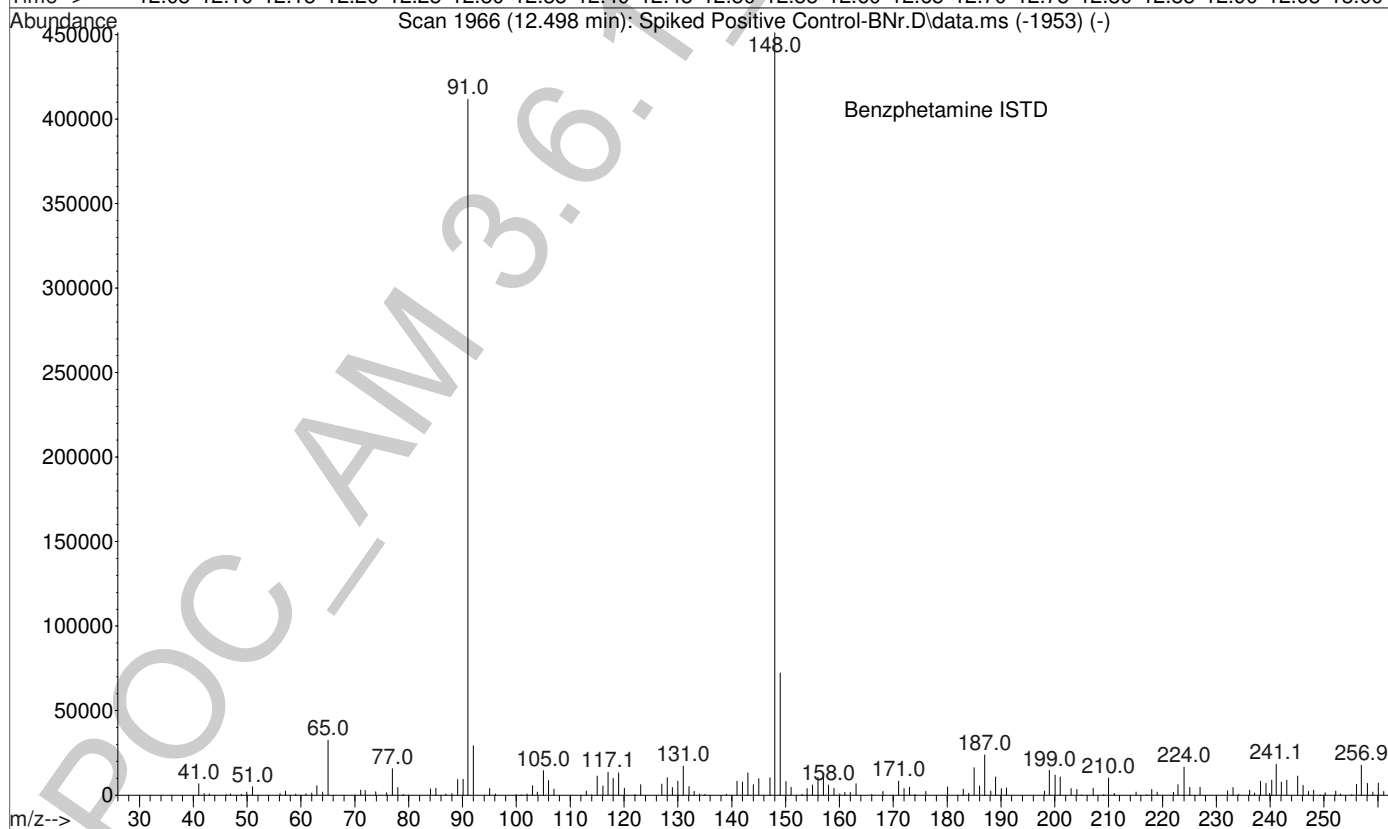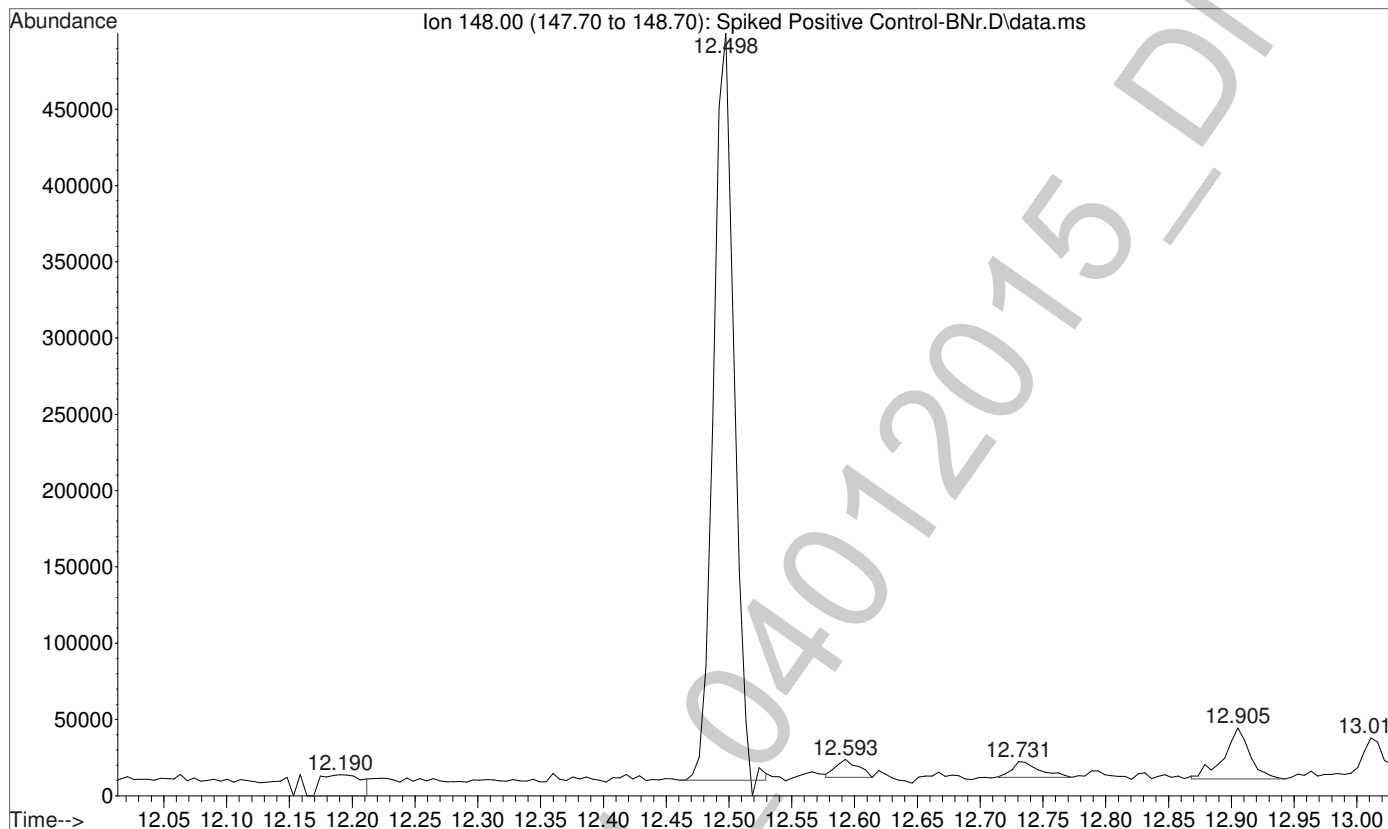



File :C:\gcms\1\data\Blood\040115BN\Reinjection Longer GC Method\S  
... piked Positive Control-BNr.D  
Operator : 5LAB-C01\ISPuser  
Instrument : Major Mass Spec  
Acquired : 02 Apr 2015 01:26 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1

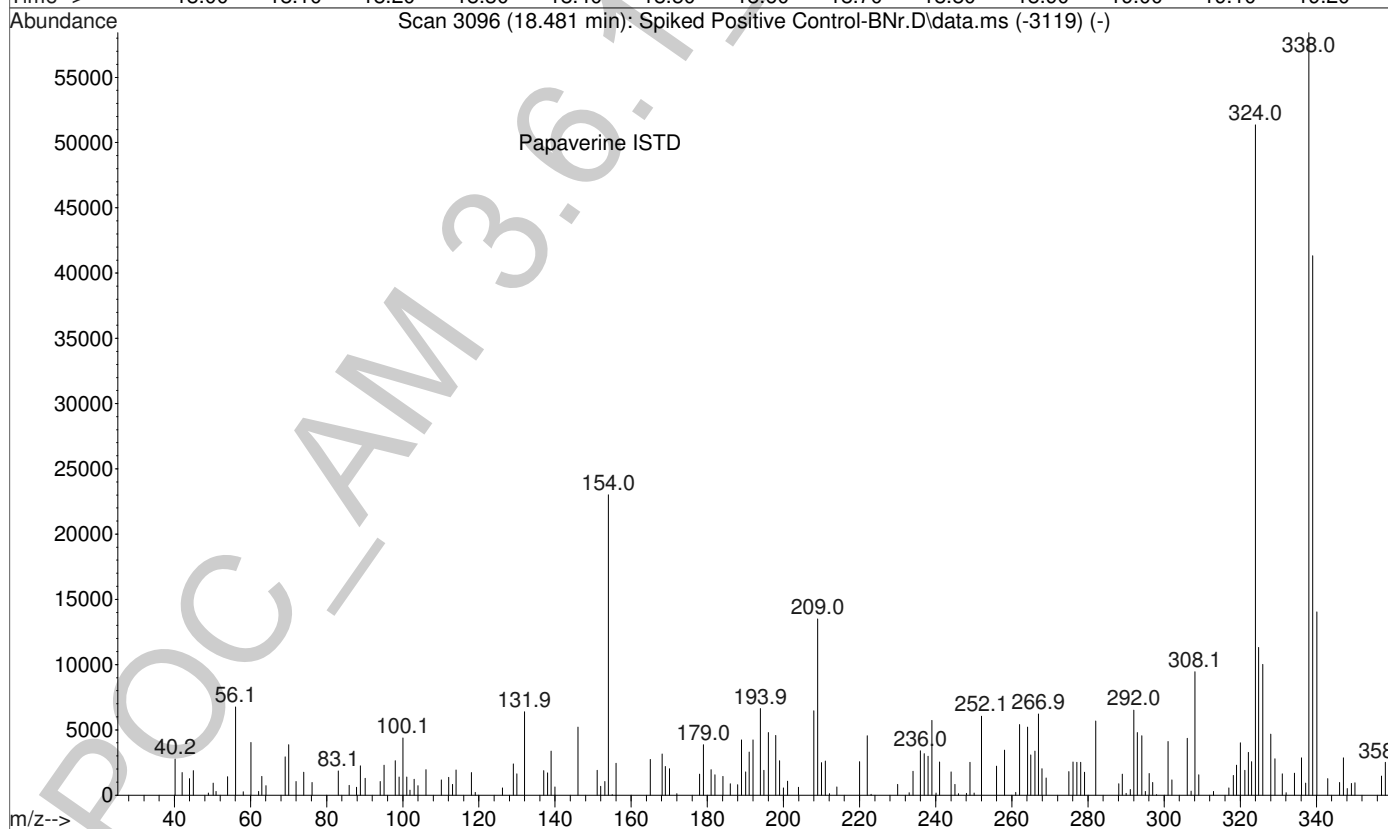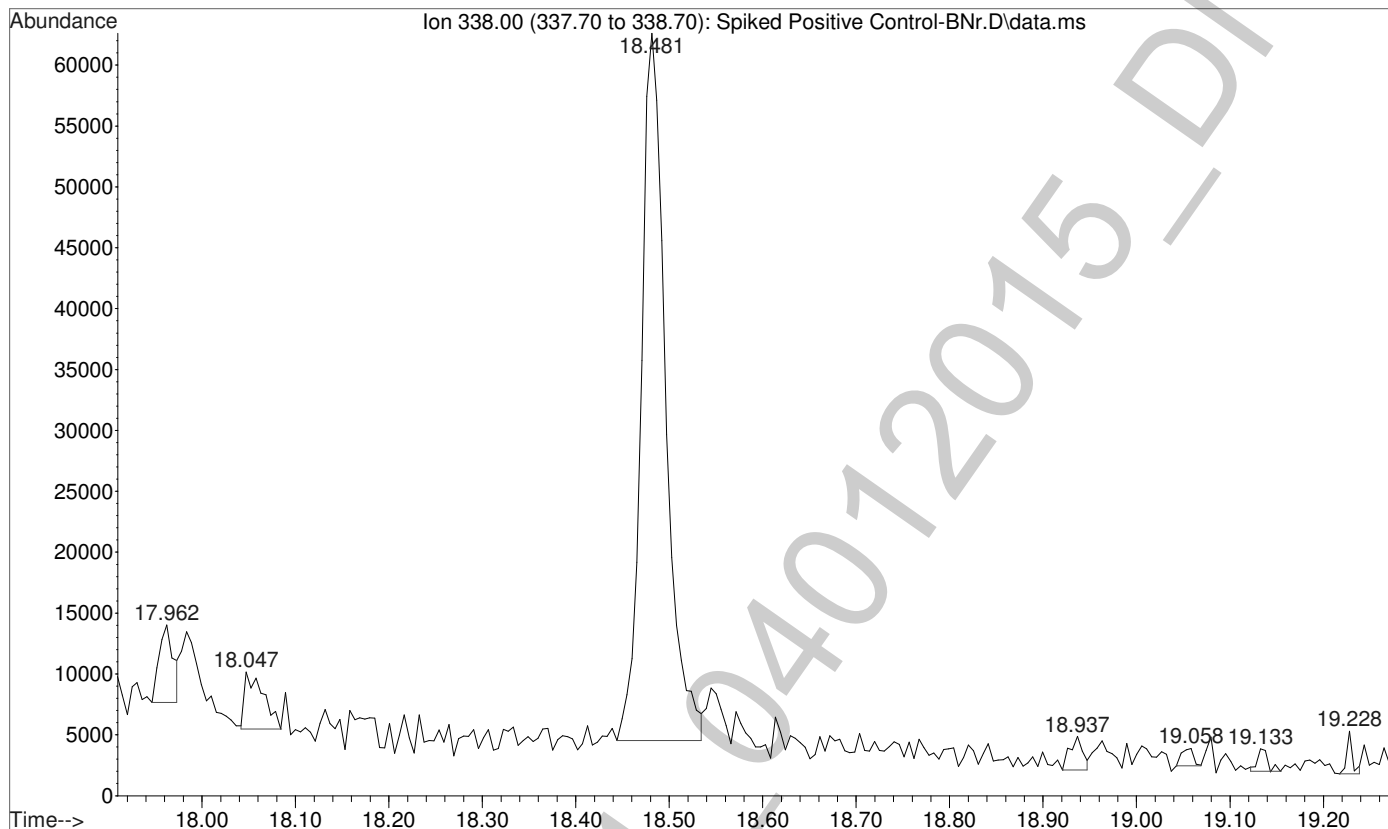



File :C:\gcms\1\data\Blood\040115BN\Reinjection Longer GC Method\S  
... piked Positive Control-BNr.D  
Operator : 5LAB-C01\ISPuser  
Instrument : Major Mass Spec  
Acquired : 02 Apr 2015 01:26 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1

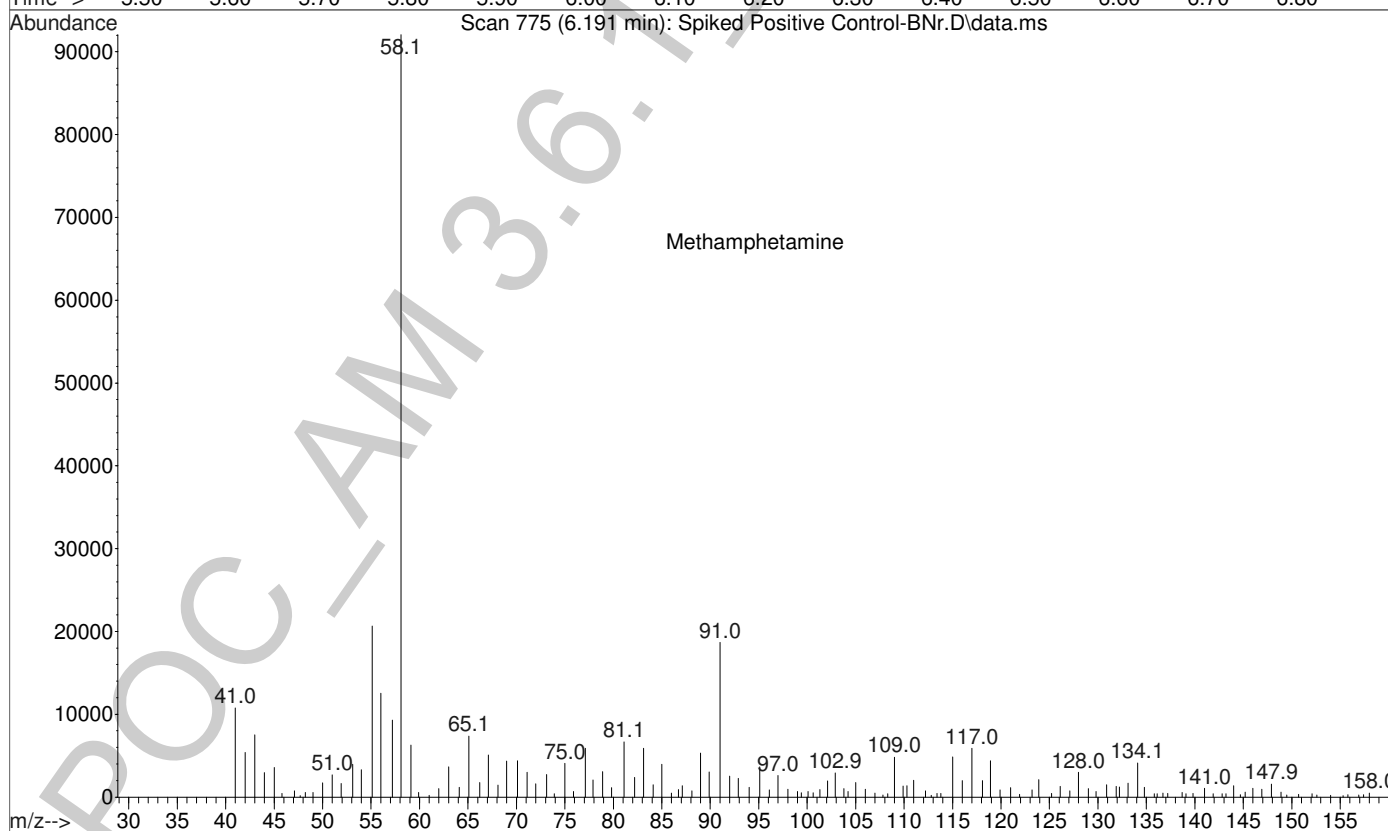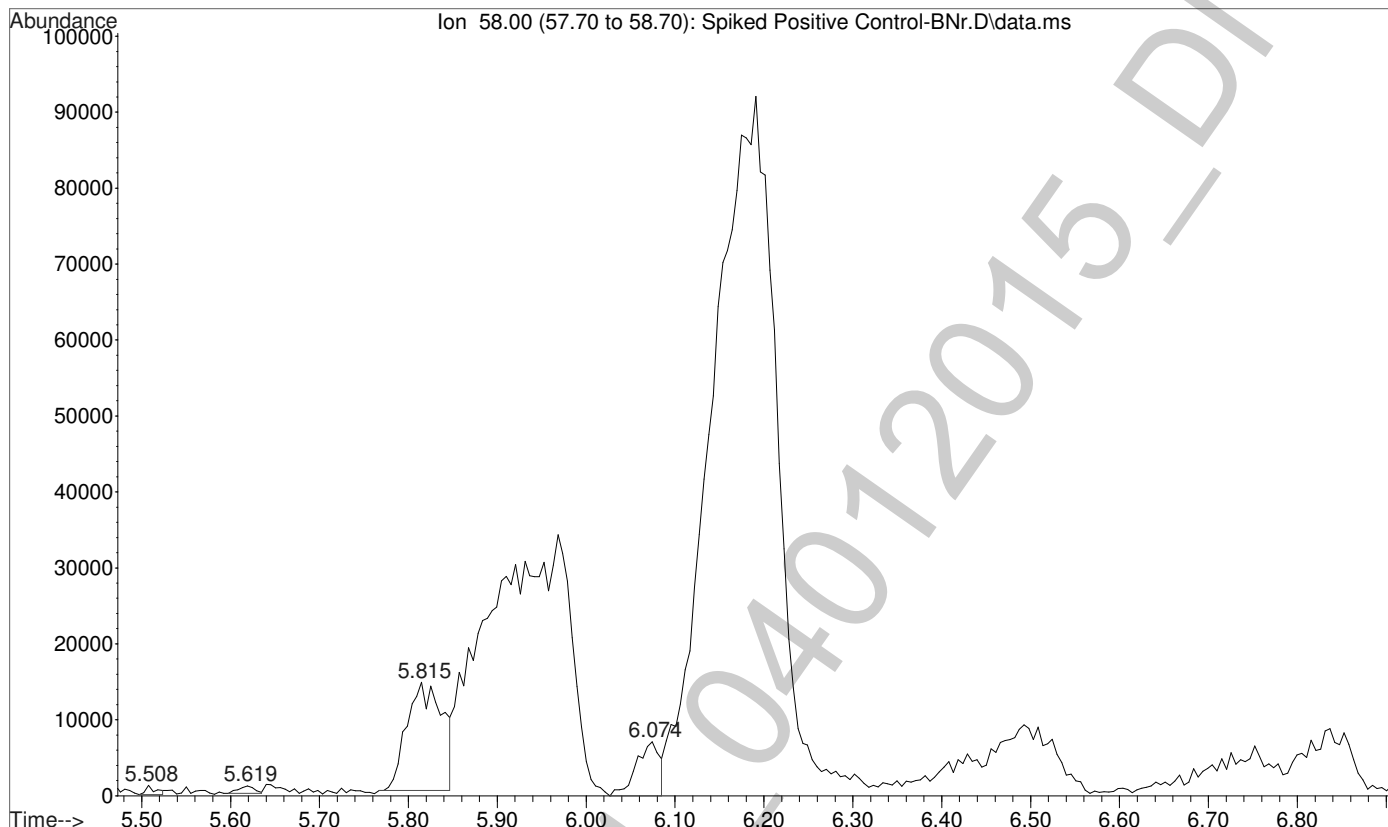

File :C:\gcms\1\data\Blood\040115BN\Reinjection Longer GC Method\S  
... piked Positive Control-BNr.D  
Operator : 5LAB-C01\ISPuser  
Instrument : Major Mass Spec  
Acquired : 02 Apr 2015 01:26 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1

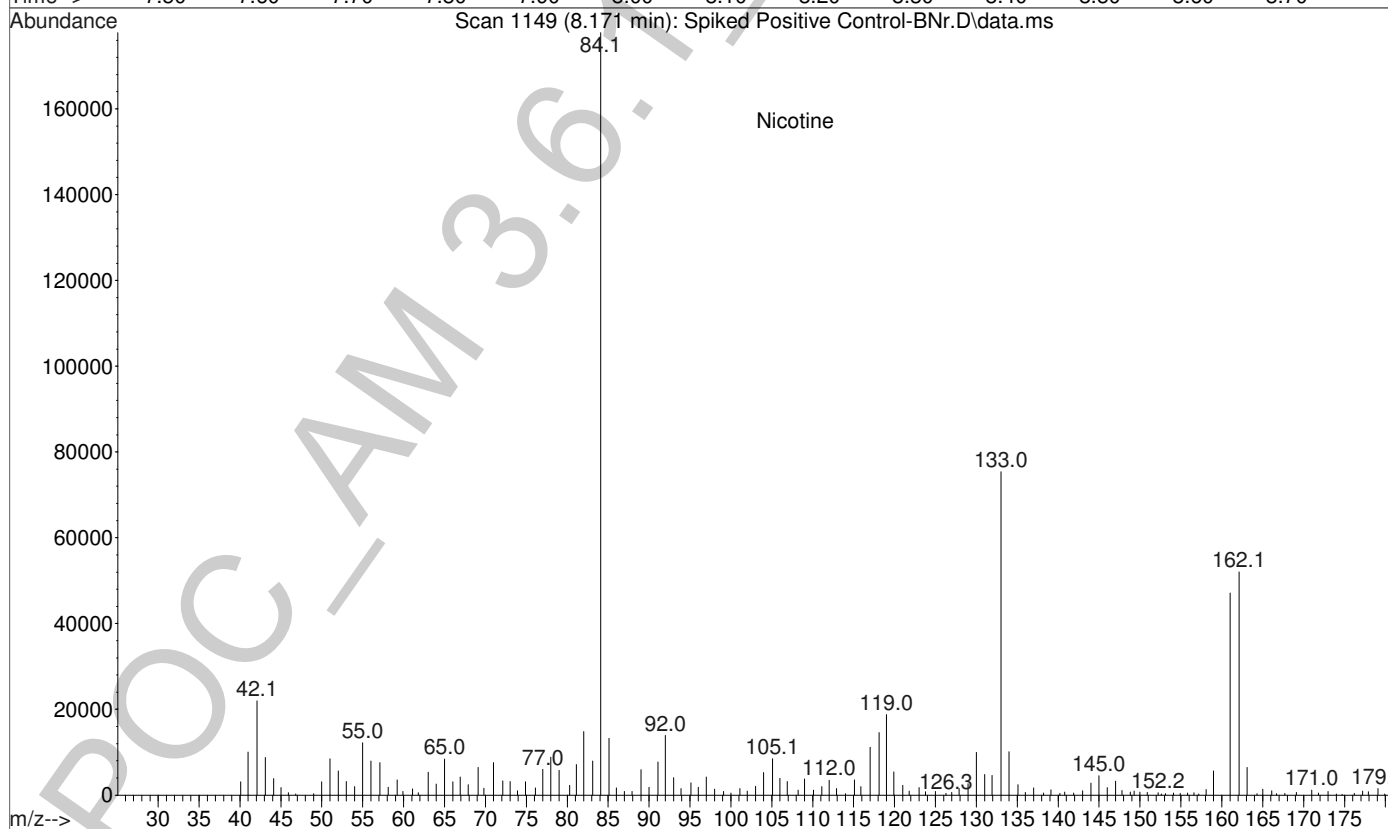
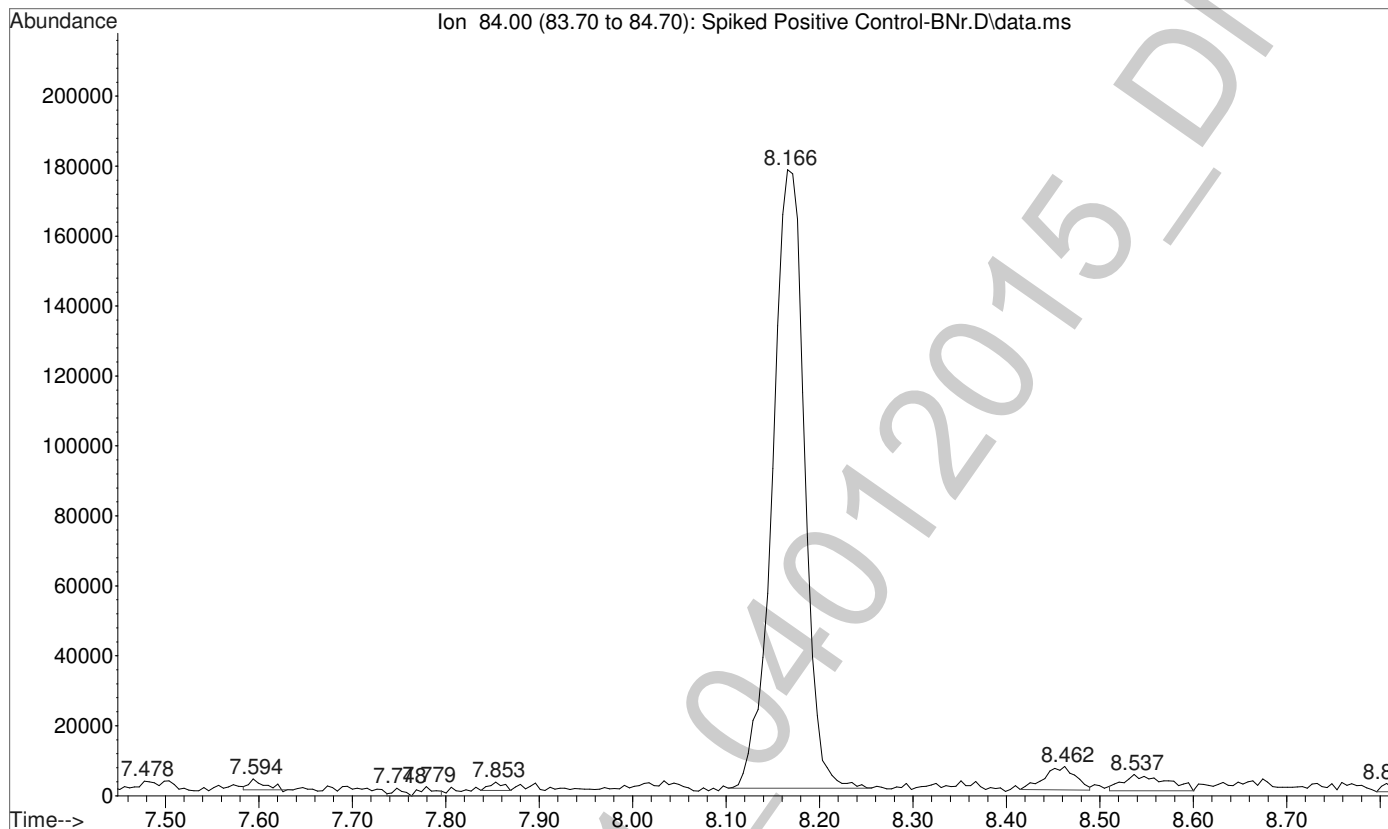


File :C:\gcms\1\data\Blood\040115BN\Reinjection Longer GC Method\S  
... piked Positive Control-BNr.D  
Operator : 5LAB-C01\ISPuser  
Instrument : Major Mass Spec  
Acquired : 02 Apr 2015 01:26 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1

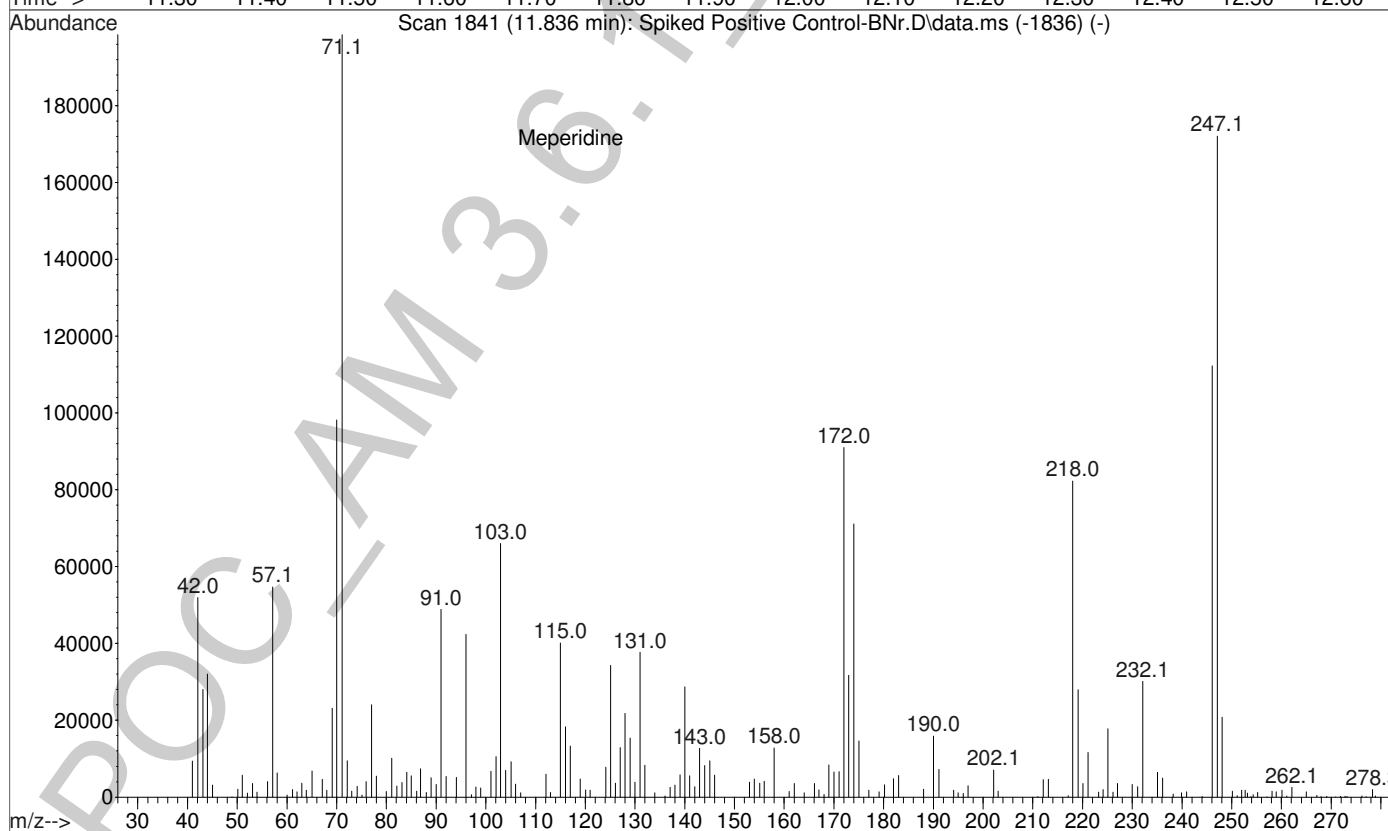
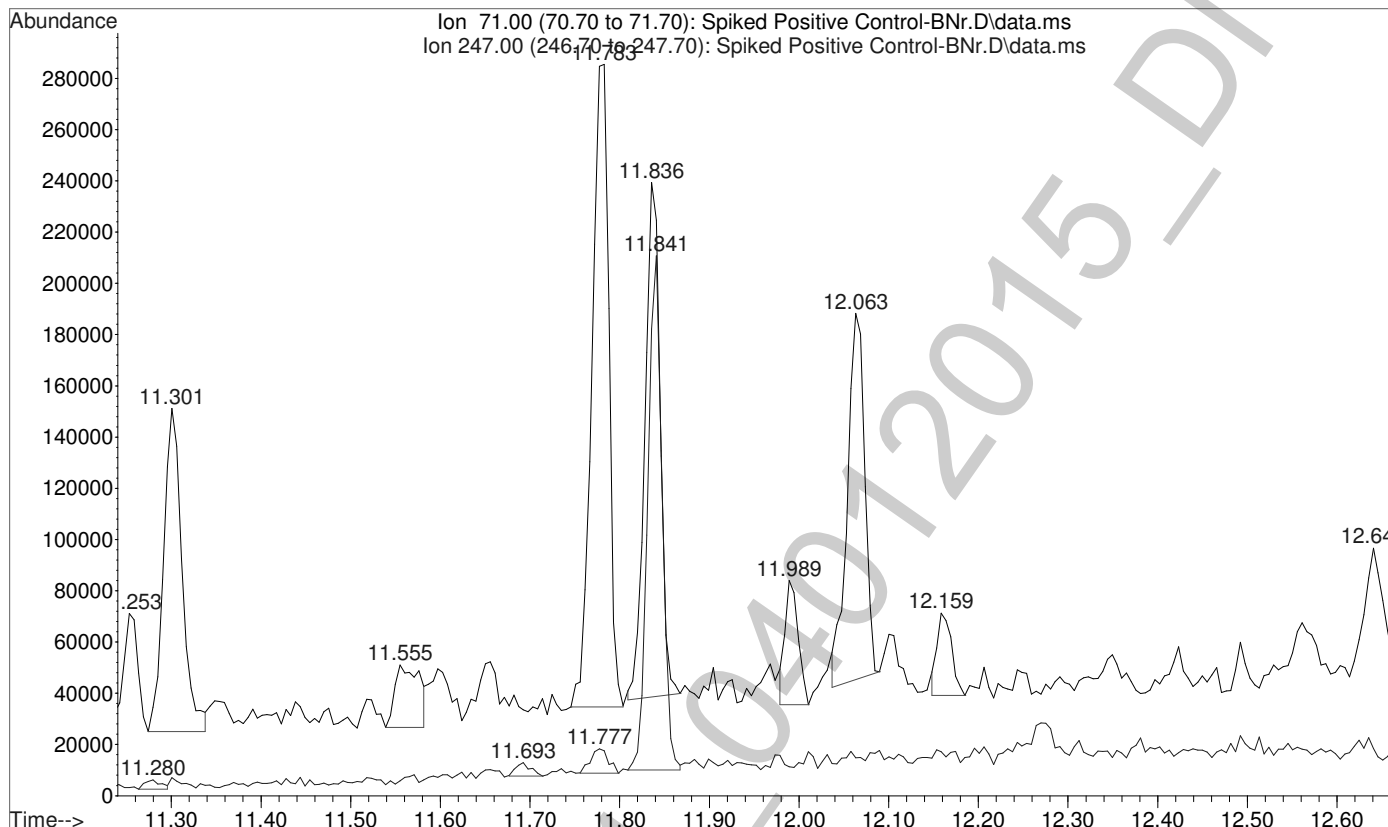






File :C:\gcms\1\data\Blood\040115BN\Reinjection Longer GC Method\S  
... piked Positive Control-BNr.D  
Operator : 5LAB-C01\ISPuser  
Instrument : Major Mass Spec  
Acquired : 02 Apr 2015 01:26 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1

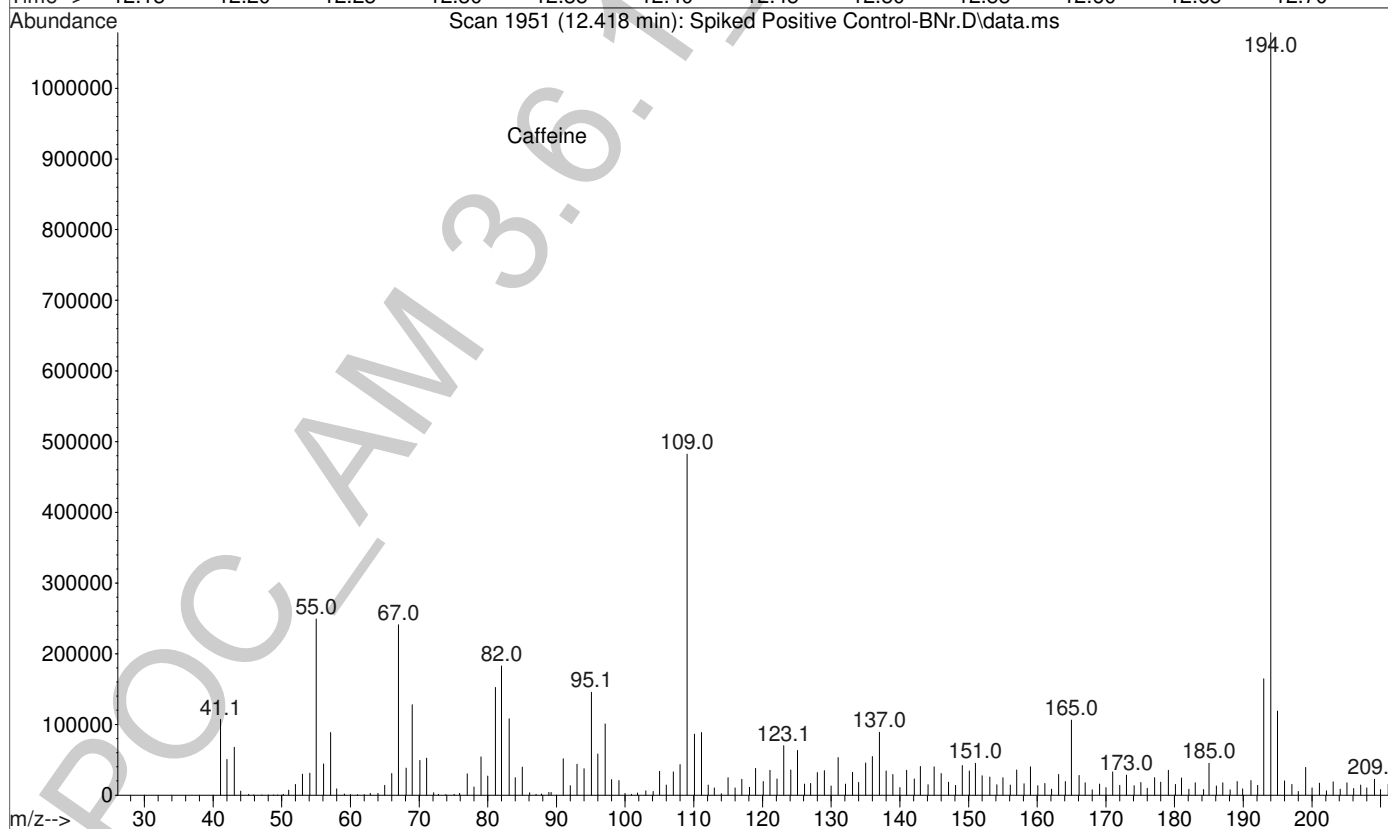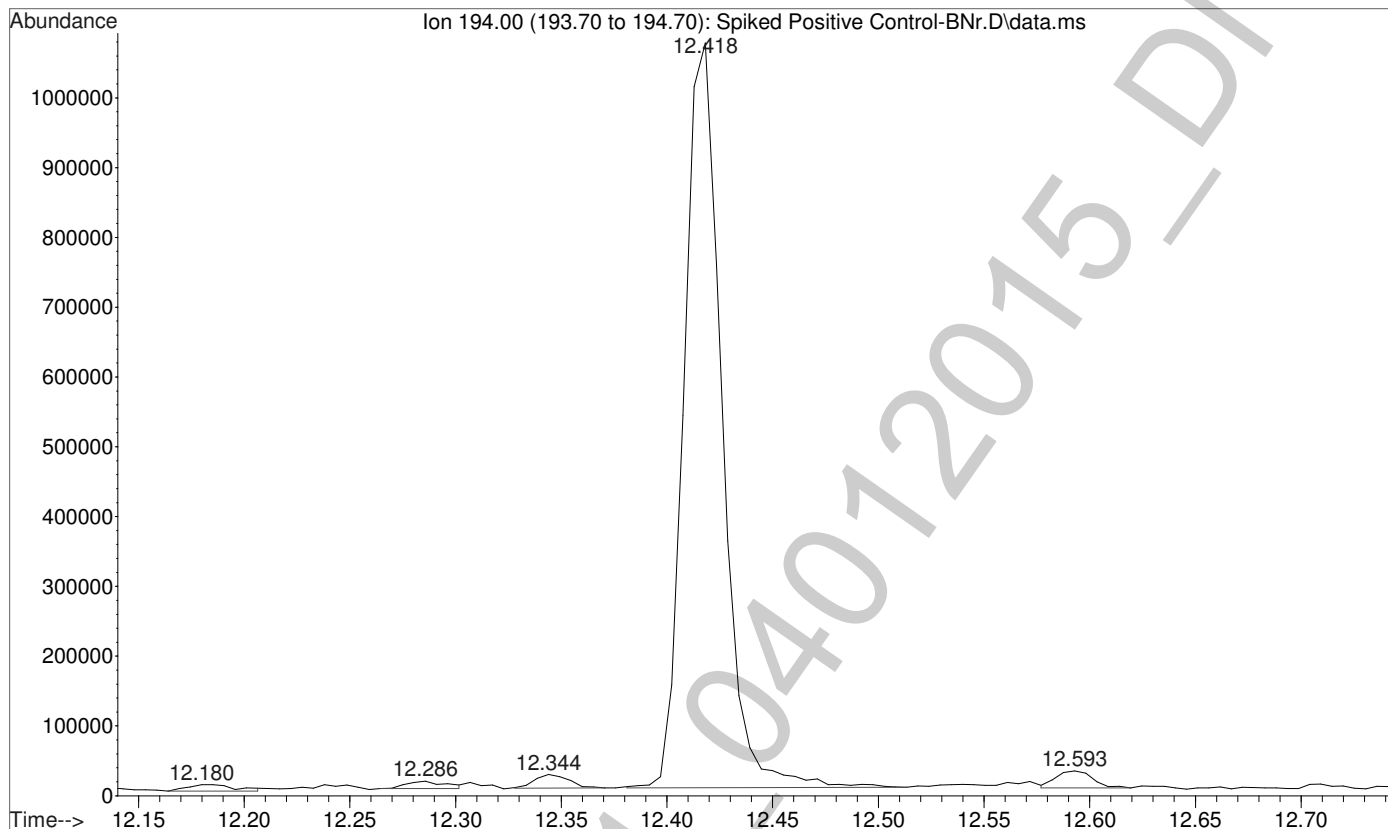



File :C:\gcms\1\data\Blood\040115BN\Reinjection Longer GC Method\S  
... piked Positive Control-BNr.D  
Operator : 5LAB-C01\ISPuser  
Instrument : Major Mass Spec  
Acquired : 02 Apr 2015 01:26 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1

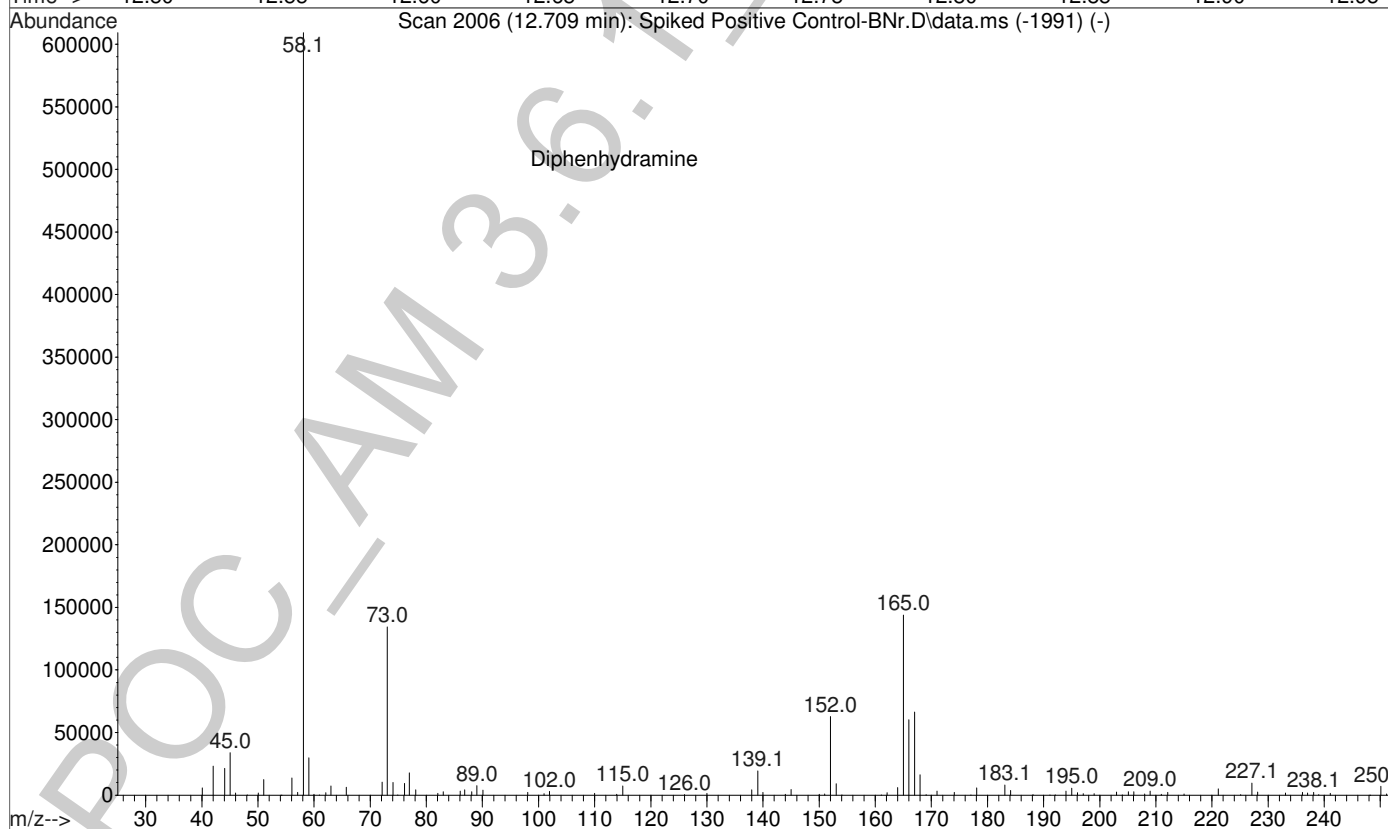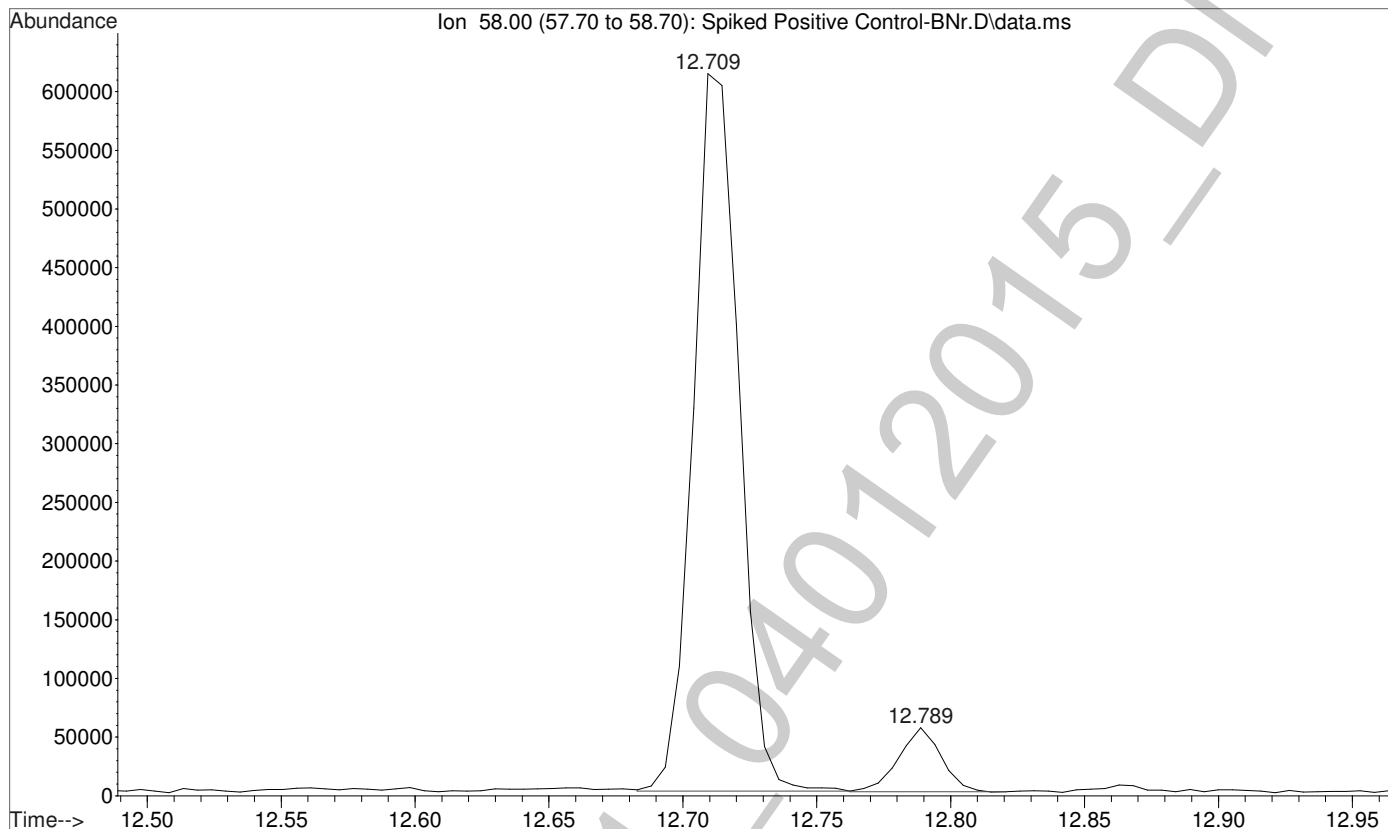



File :C:\gcms\1\data\Blood\040115BN\Reinjection Longer GC Method\S  
... piked Positive Control-BNr.D  
Operator : 5LAB-C01\ISPuser  
Instrument : Major Mass Spec  
Acquired : 02 Apr 2015 01:26 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1

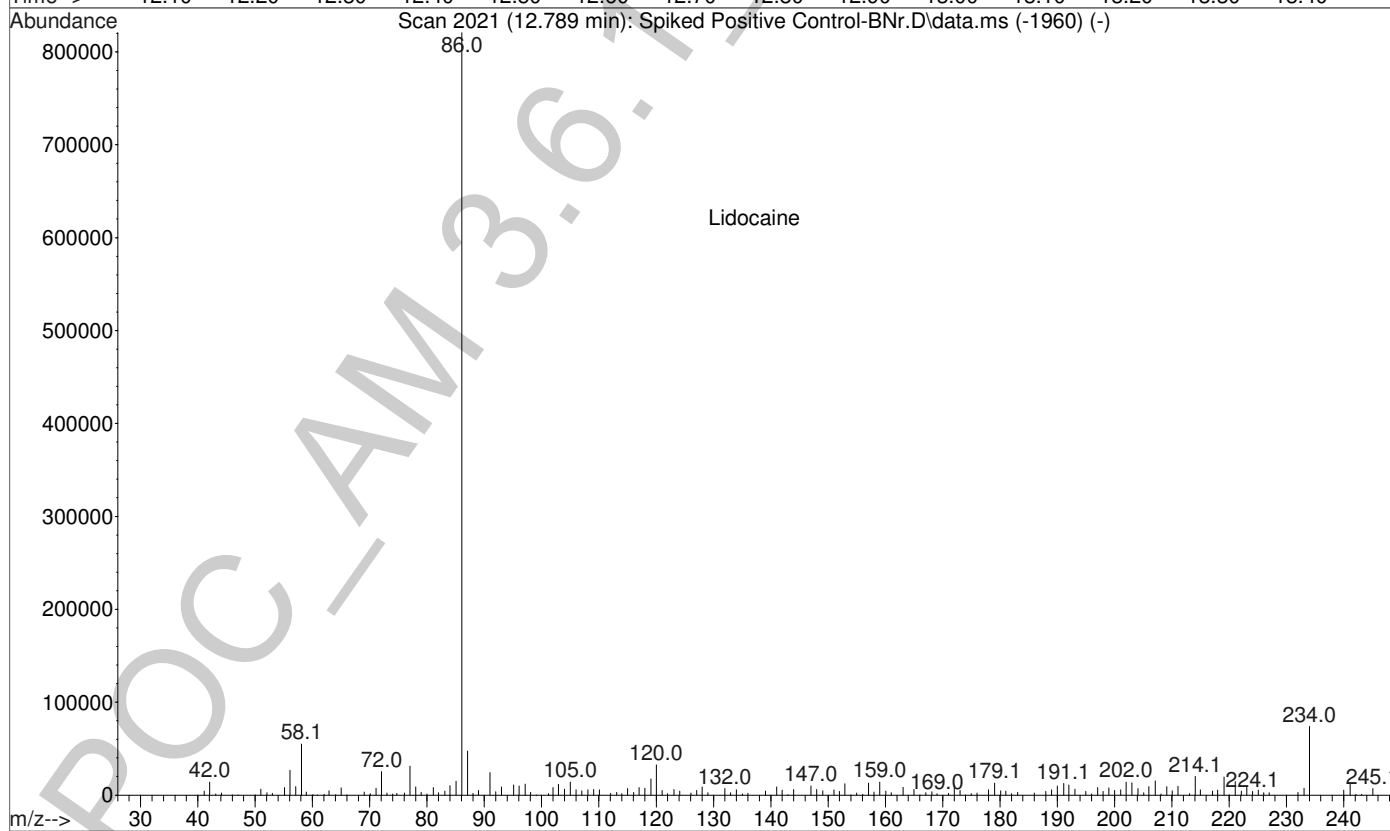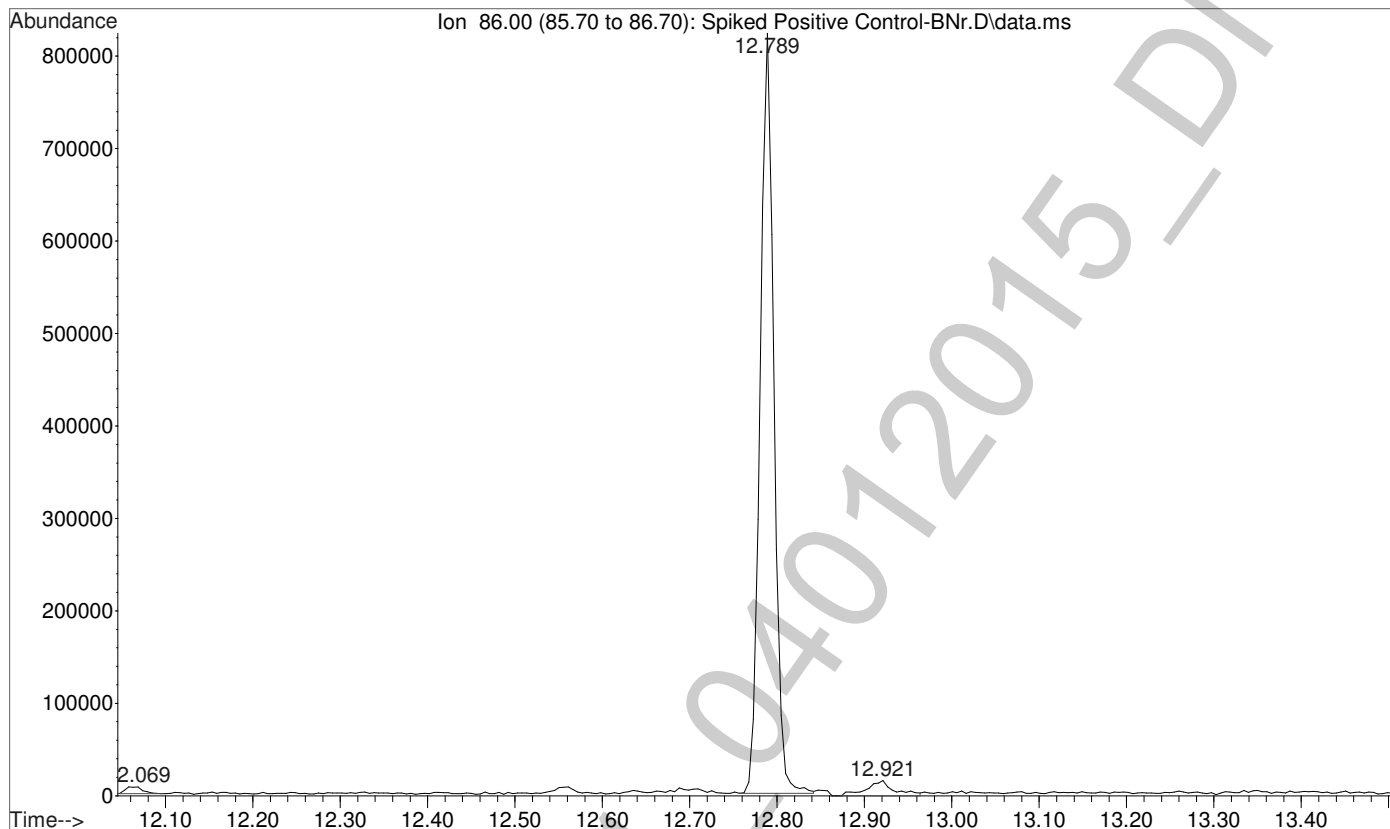



File :C:\gcms\1\data\Blood\040115BN\Reinjection Longer GC Method\S  
... piked Positive Control-BNr.D  
Operator : 5LAB-C01\ISPuser  
Instrument : Major Mass Spec  
Acquired : 02 Apr 2015 01:26 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1

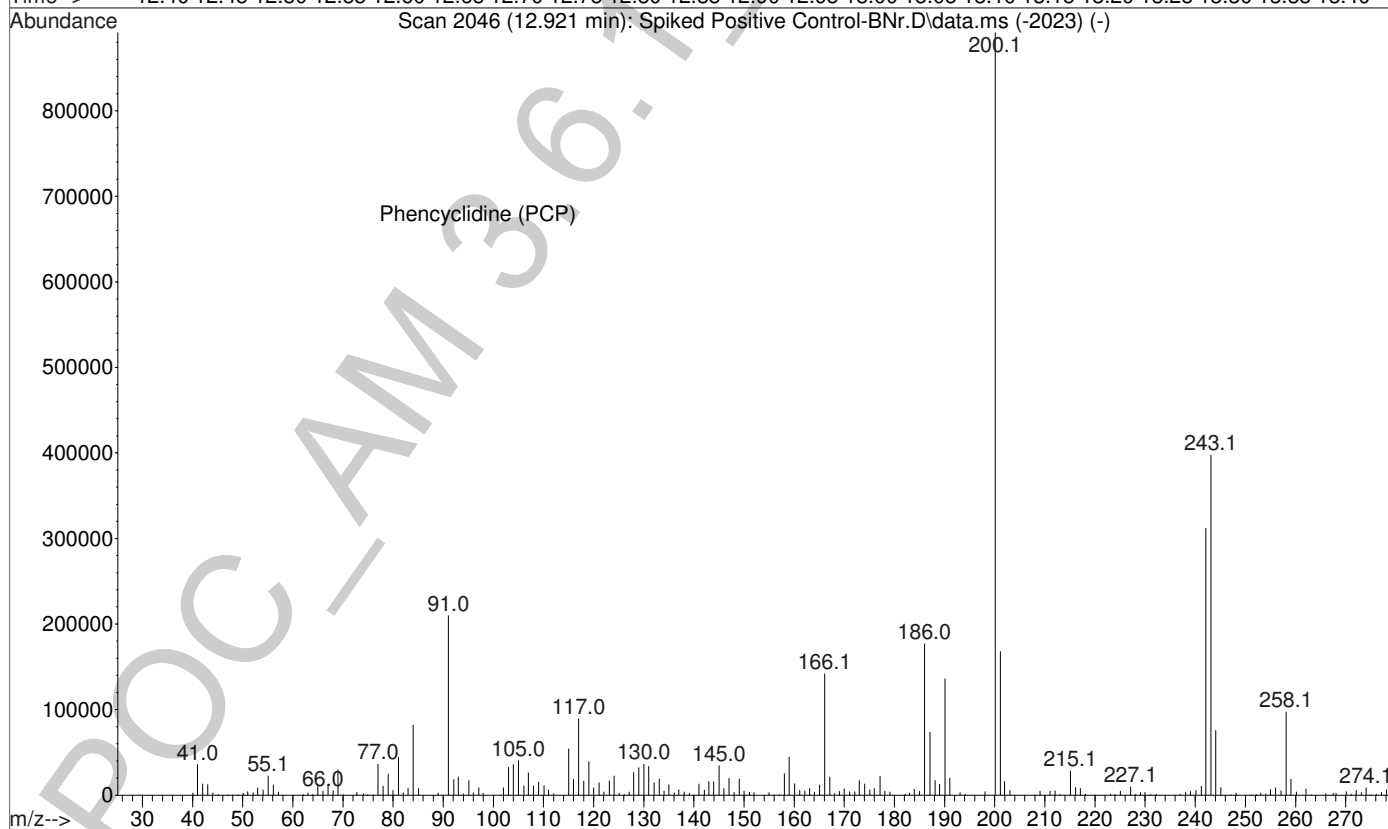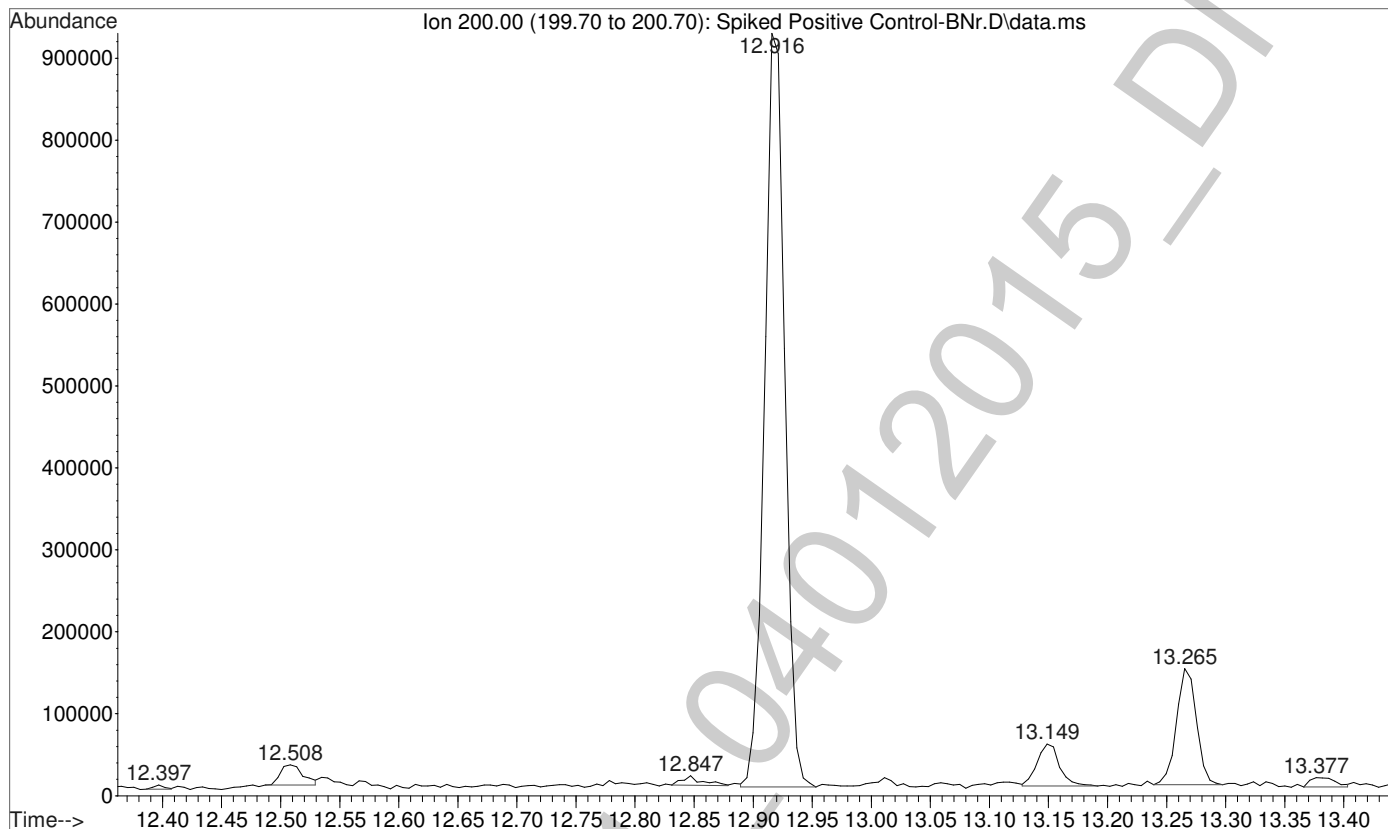



File :C:\gcms\1\data\Blood\040115BN\Reinjection Longer GC Method\S  
... piked Positive Control-BNr.D  
Operator : 5LAB-C01\ISPuser  
Instrument : Major Mass Spec  
Acquired : 02 Apr 2015 01:26 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1

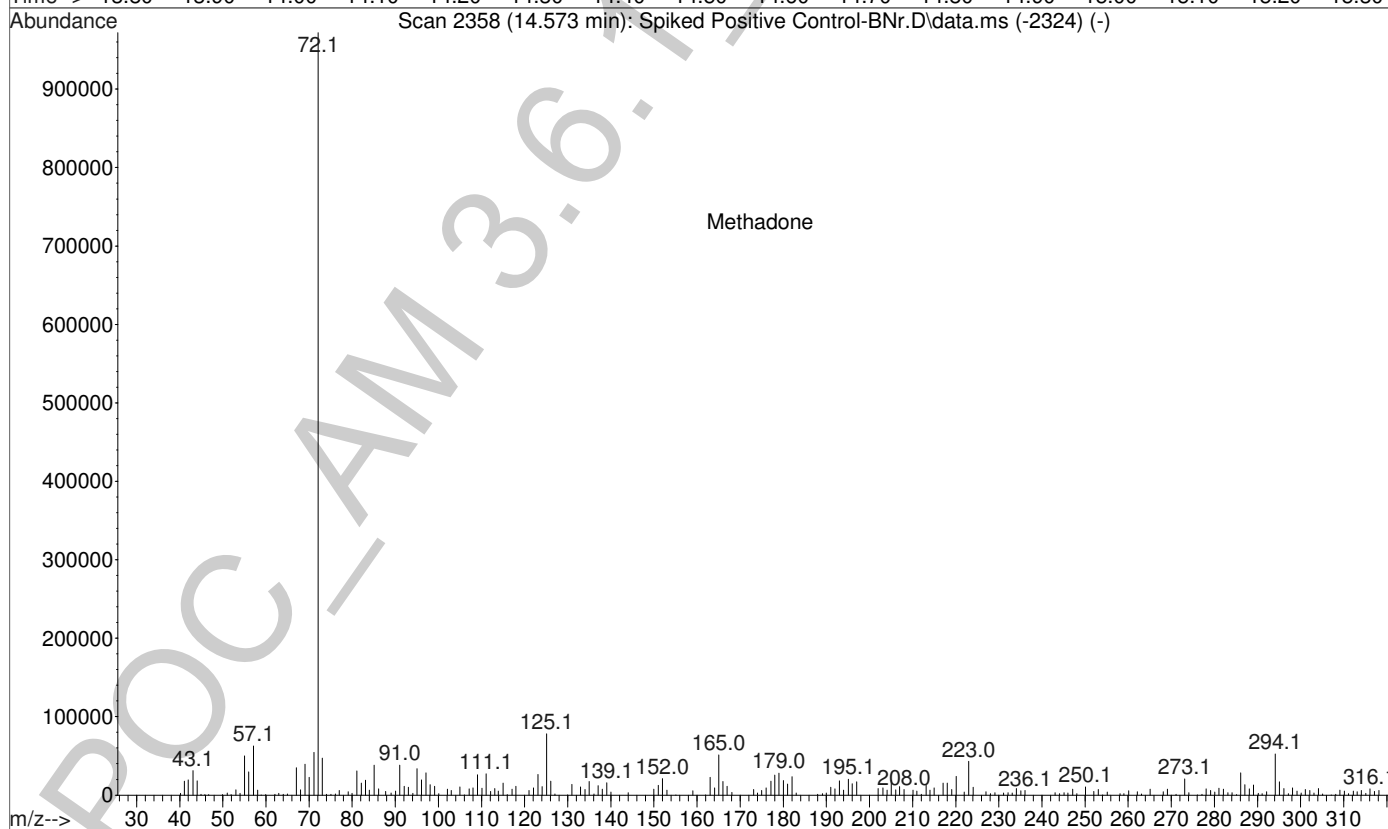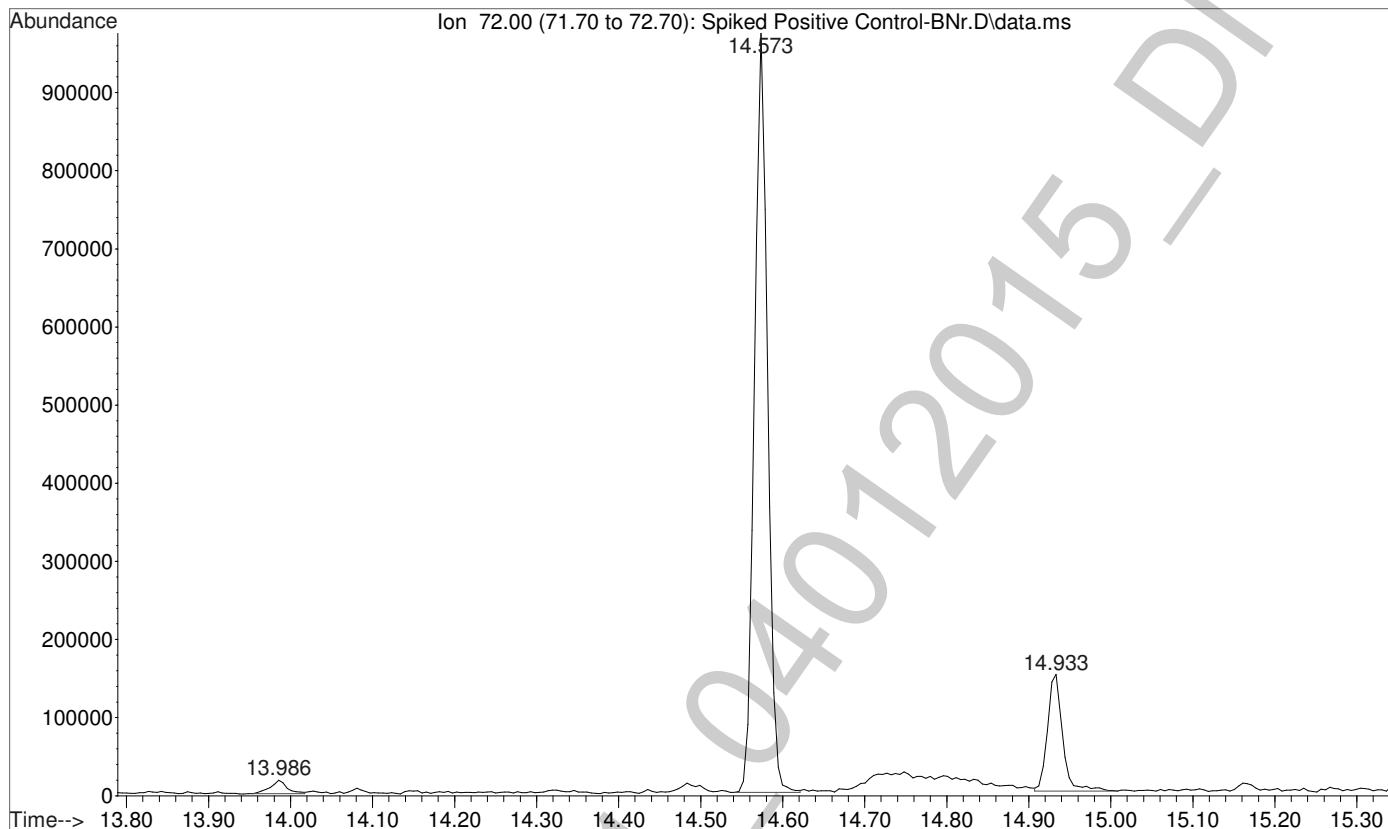



File :C:\gcms\1\data\Blood\040115BN\Reinjection Longer GC Method\S  
... piked Positive Control-BNr.D  
Operator : 5LAB-C01\ISPuser  
Instrument : Major Mass Spec  
Acquired : 02 Apr 2015 01:26 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1

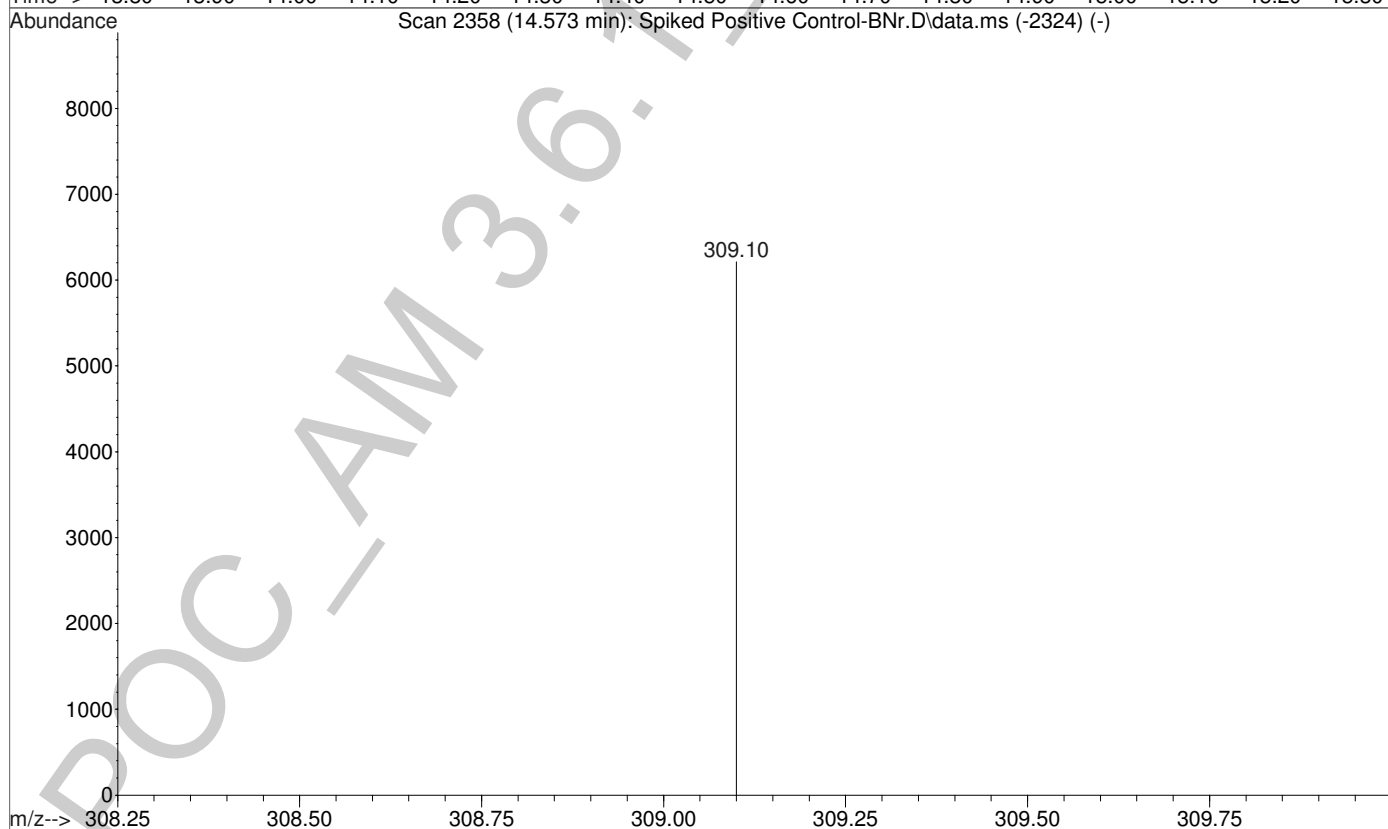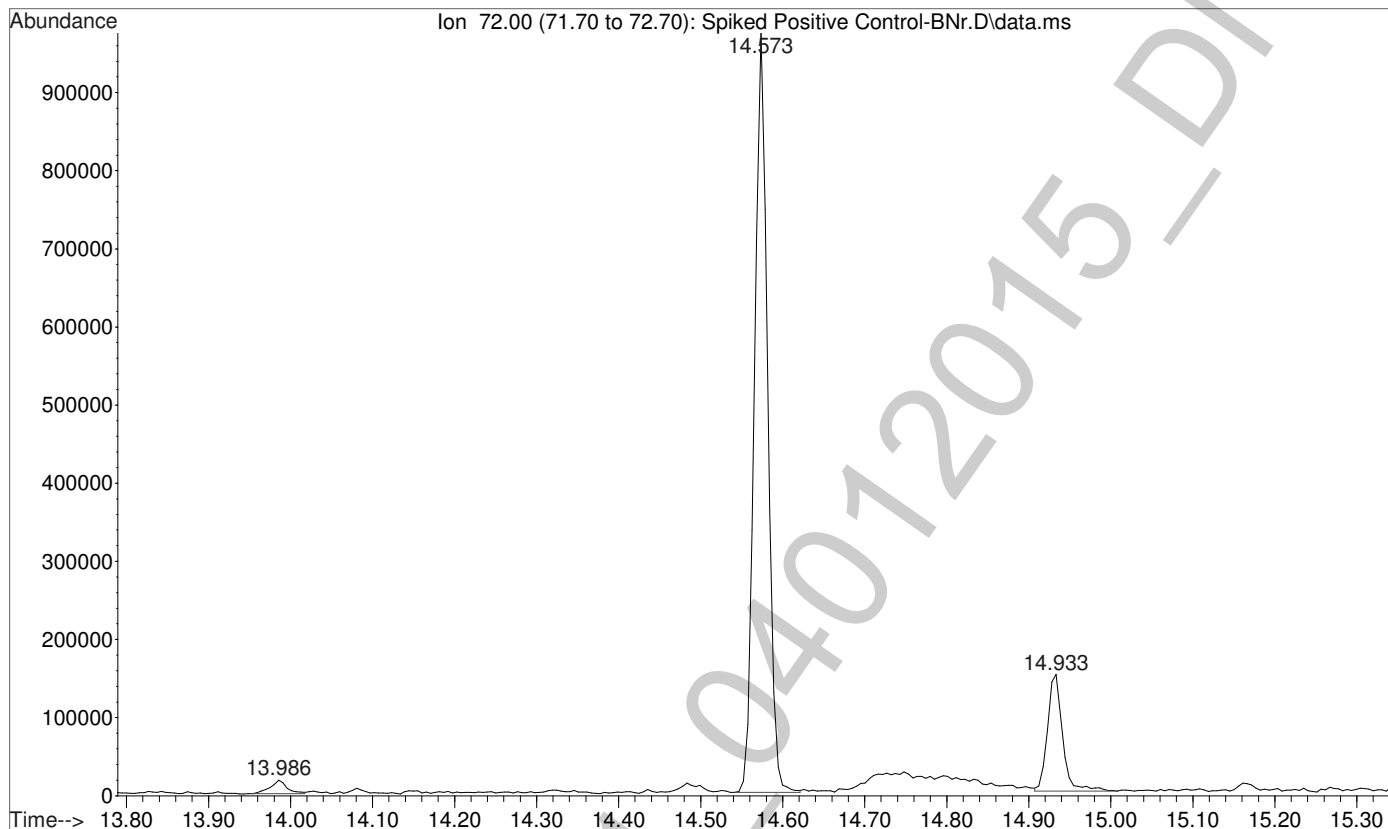

File :C:\gcms\1\data\Blood\040115BN\Reinjection Longer GC Method\S  
... piked Positive Control-BNr.D  
Operator : 5LAB-C01\ISPuser  
Instrument : Major Mass Spec  
Acquired : 02 Apr 2015 01:26 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1

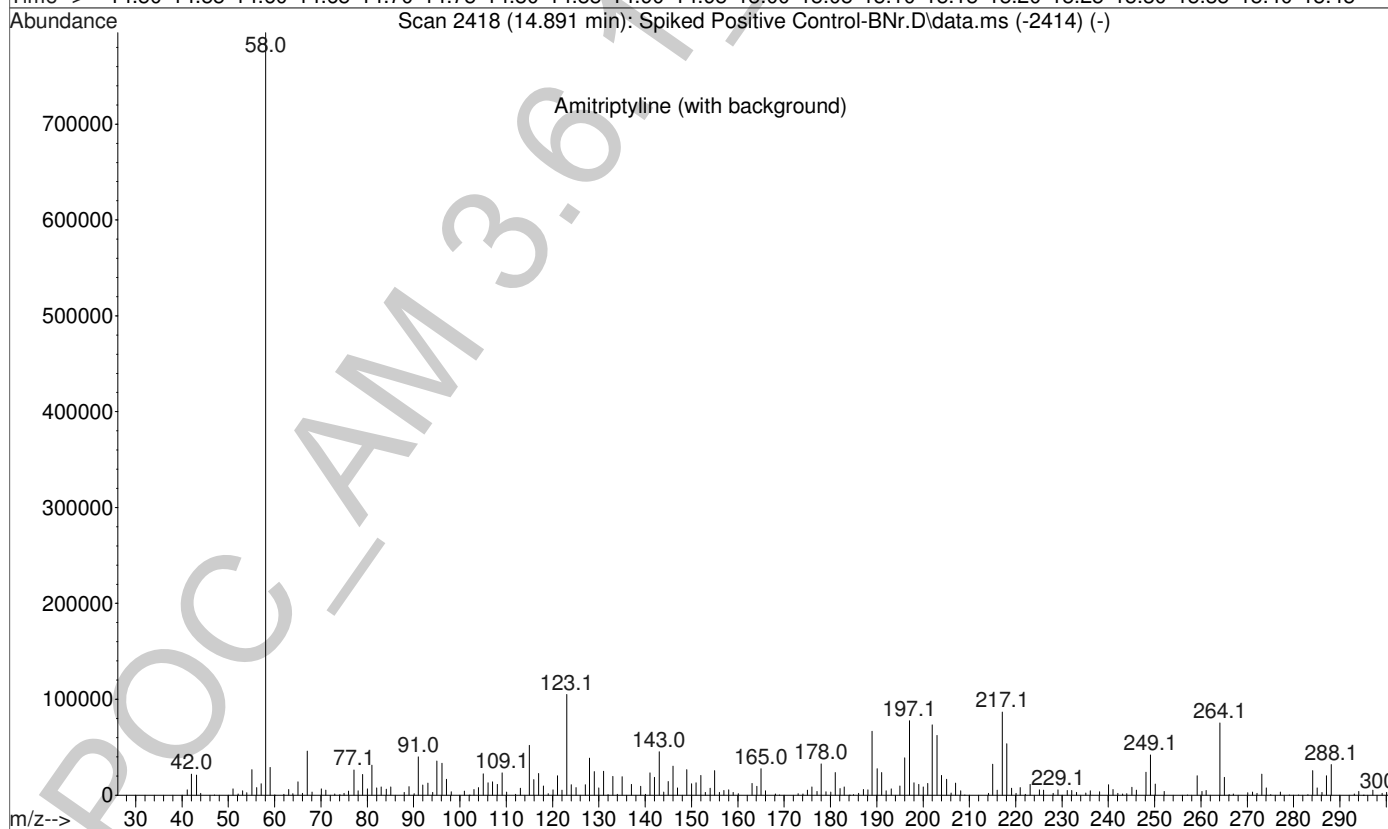
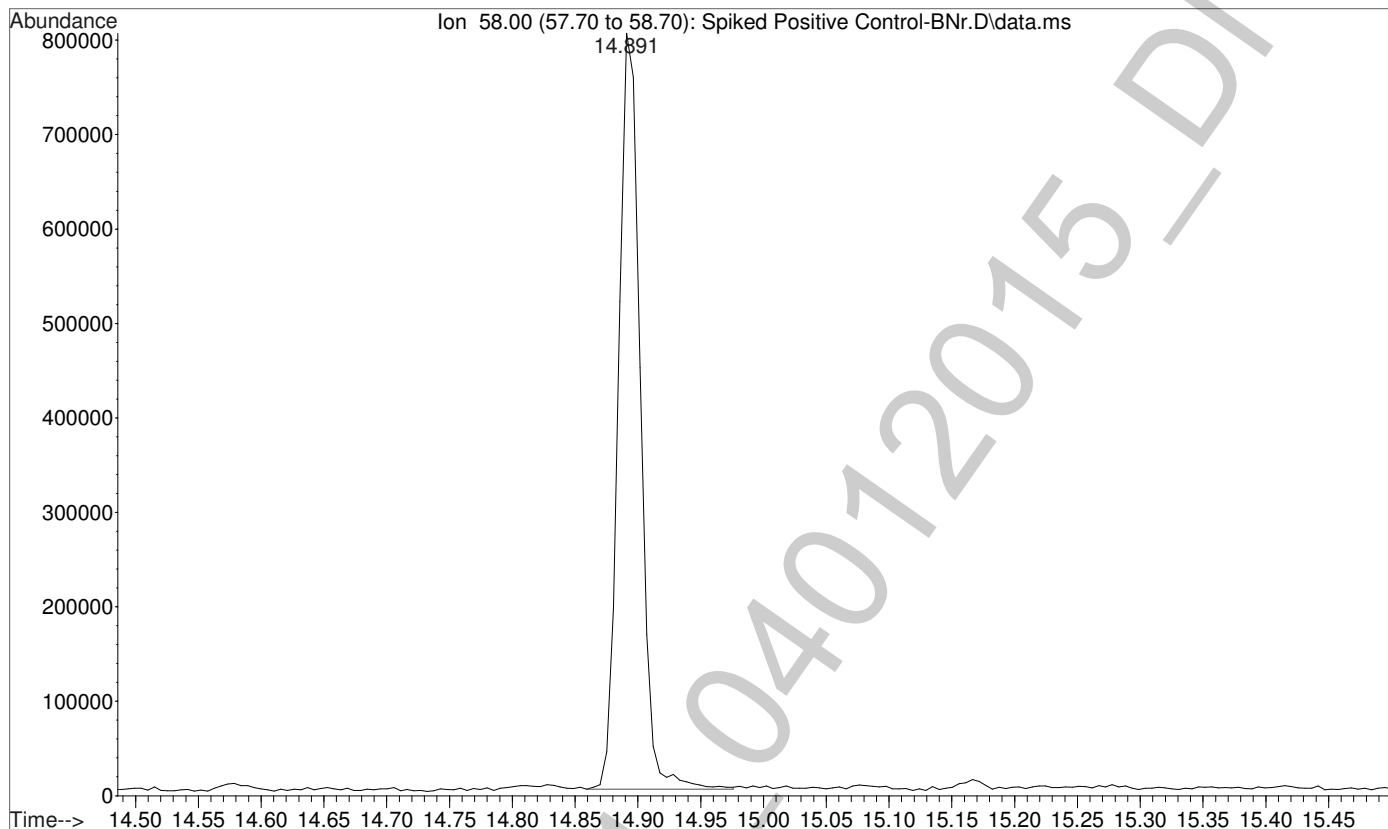


File :C:\gcms\1\data\Blood\040115BN\Reinjection Longer GC Method\S  
... piked Positive Control-BNr.D  
Operator : 5LAB-C01\ISPuser  
Instrument : Major Mass Spec  
Acquired : 02 Apr 2015 01:26 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1

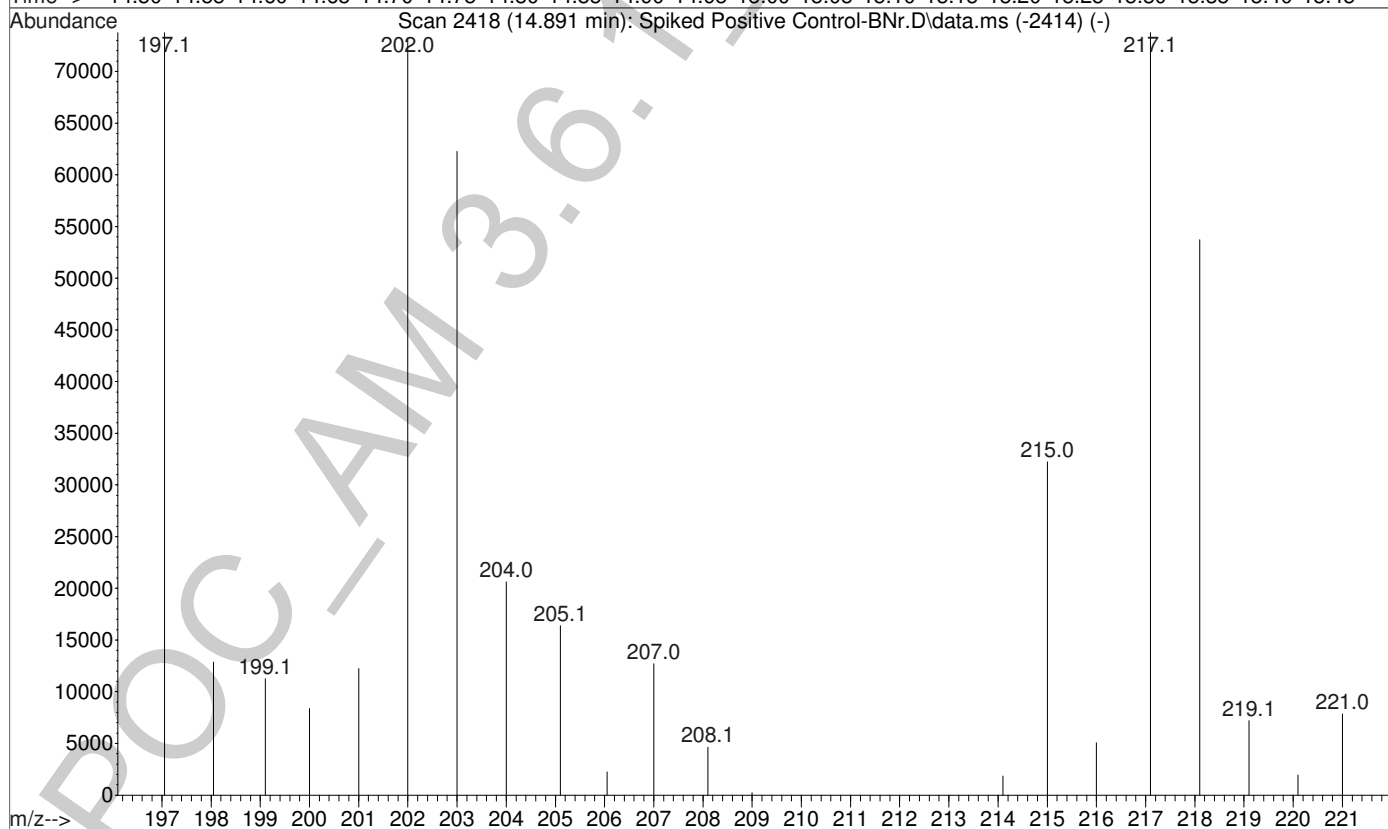
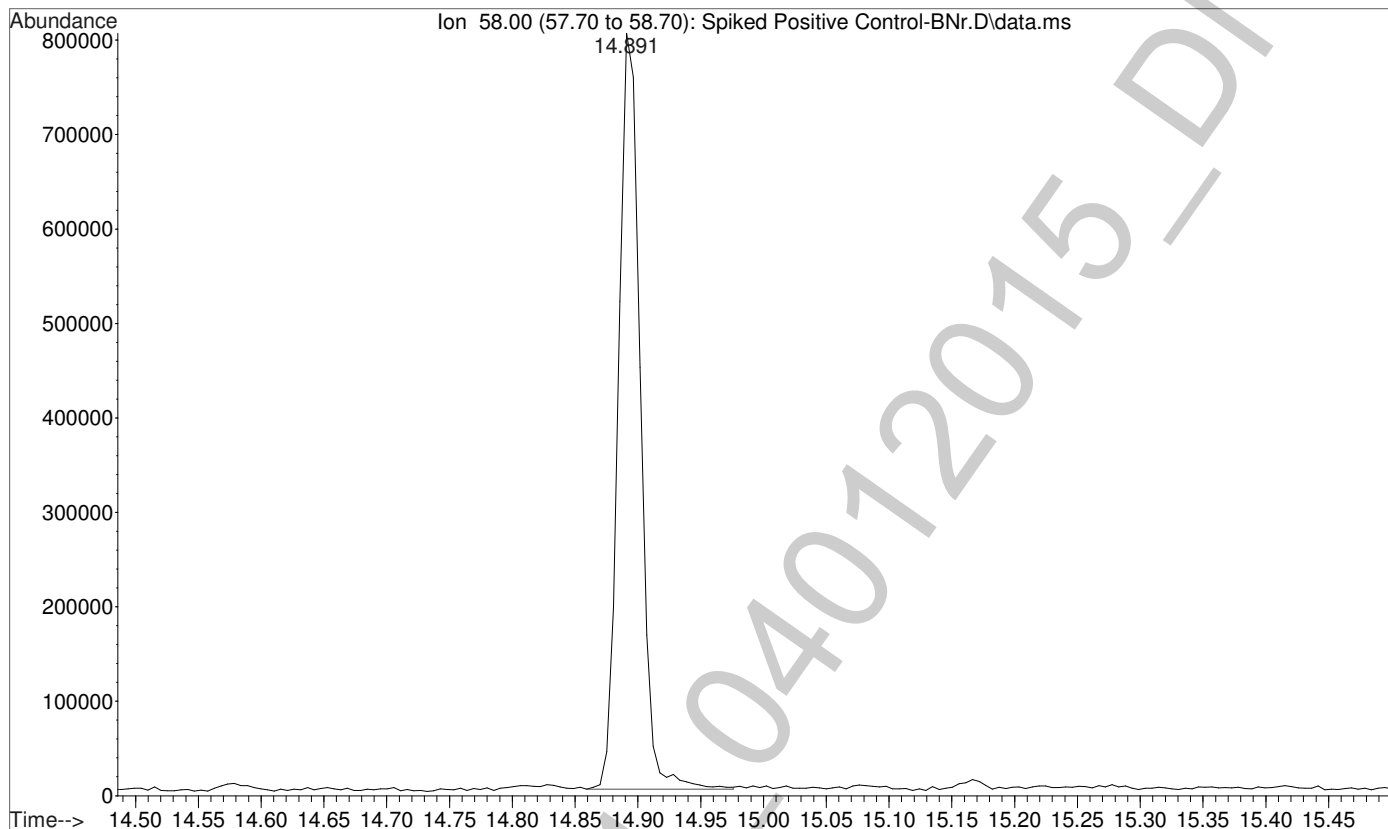






File :C:\gcms\1\data\Blood\040115BN\Reinjection Longer GC Method\S  
... piked Positive Control-BNr.D  
Operator : 5LAB-C01\ISPuser  
Instrument : Major Mass Spec  
Acquired : 02 Apr 2015 01:26 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1

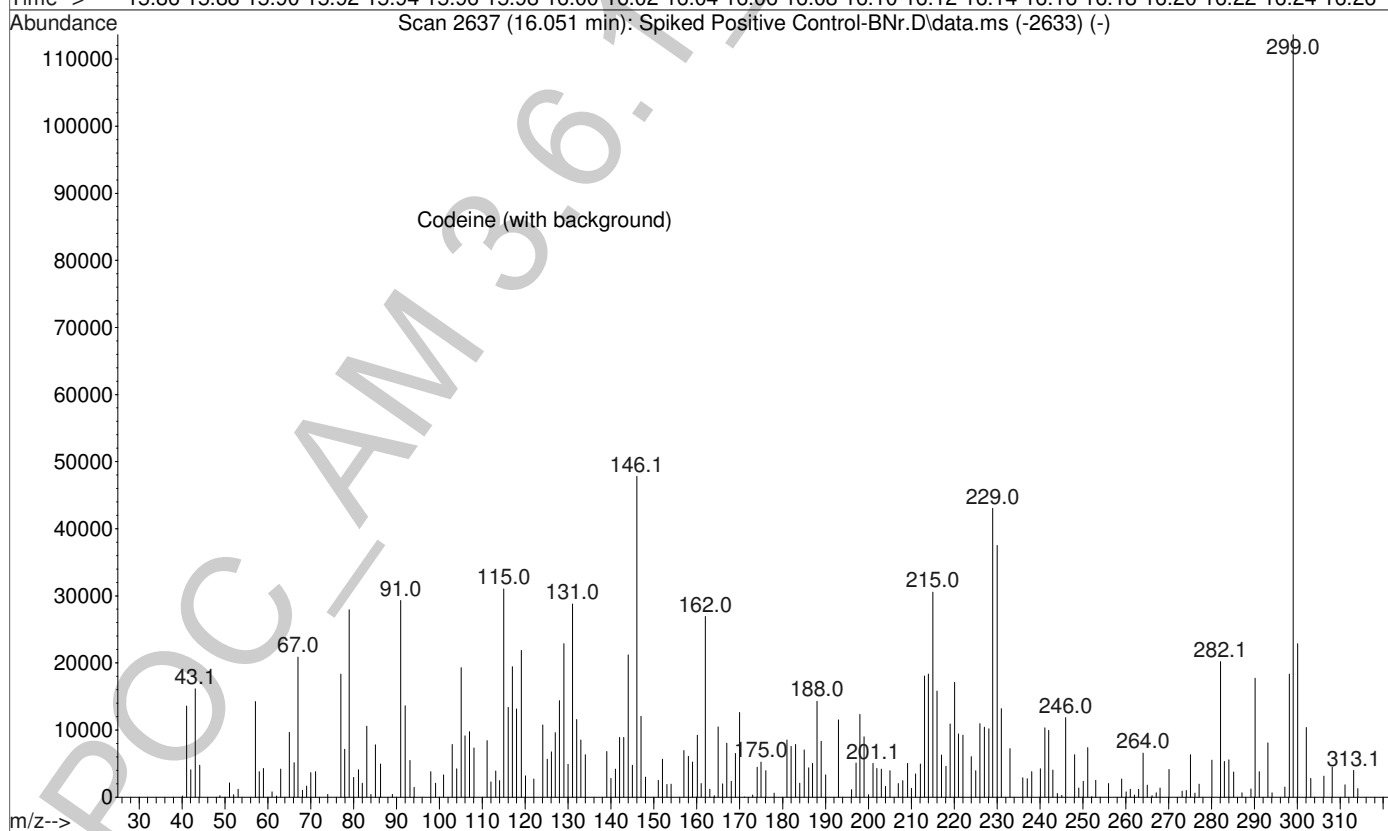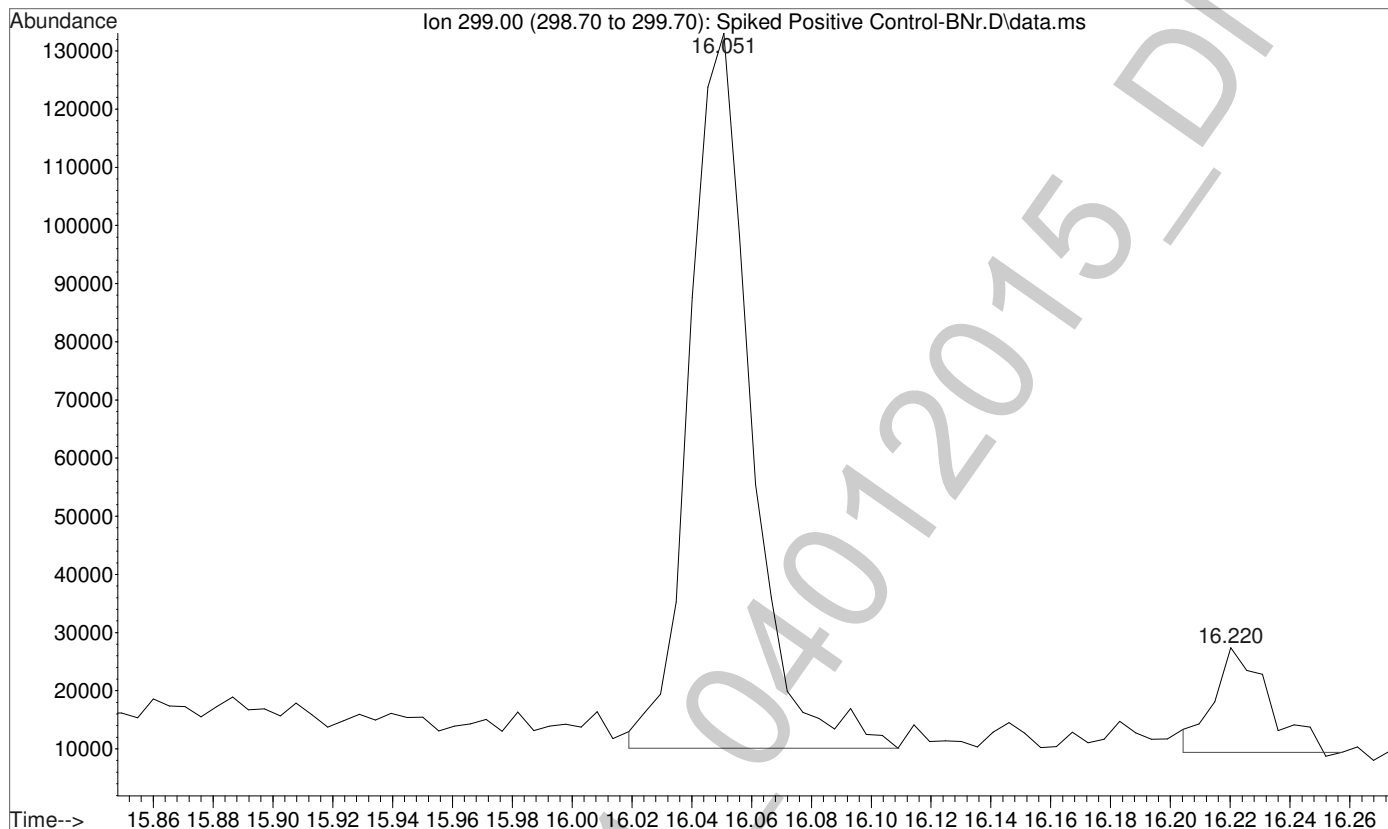



File :C:\gcms\1\data\Blood\040115BN\Reinjection Longer GC Method\S  
... piked Positive Control-BNr.D  
Operator : 5LAB-C01\ISPuser  
Instrument : Major Mass Spec  
Acquired : 02 Apr 2015 01:26 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Positive Control  
Misc Info : Analytical Method 3.6.1

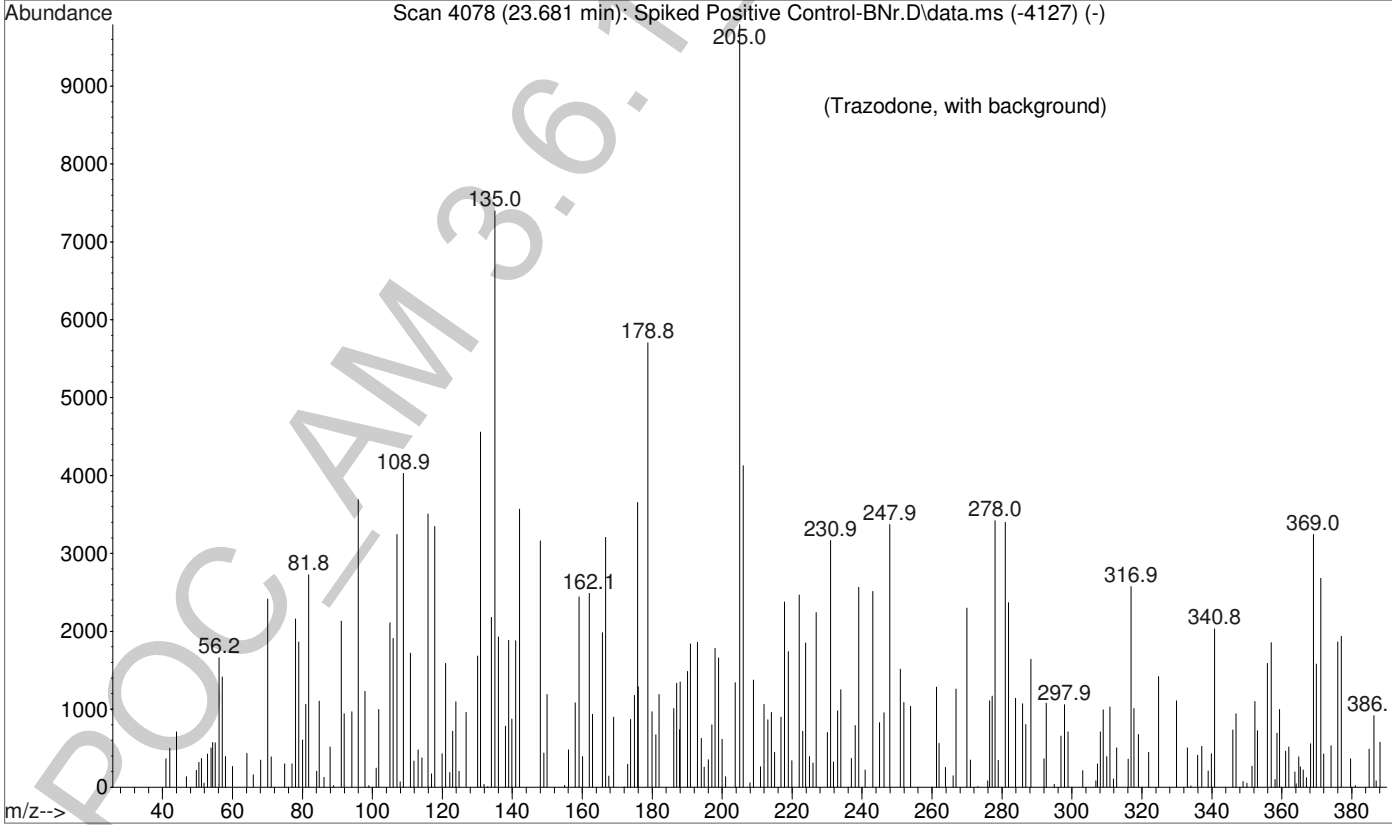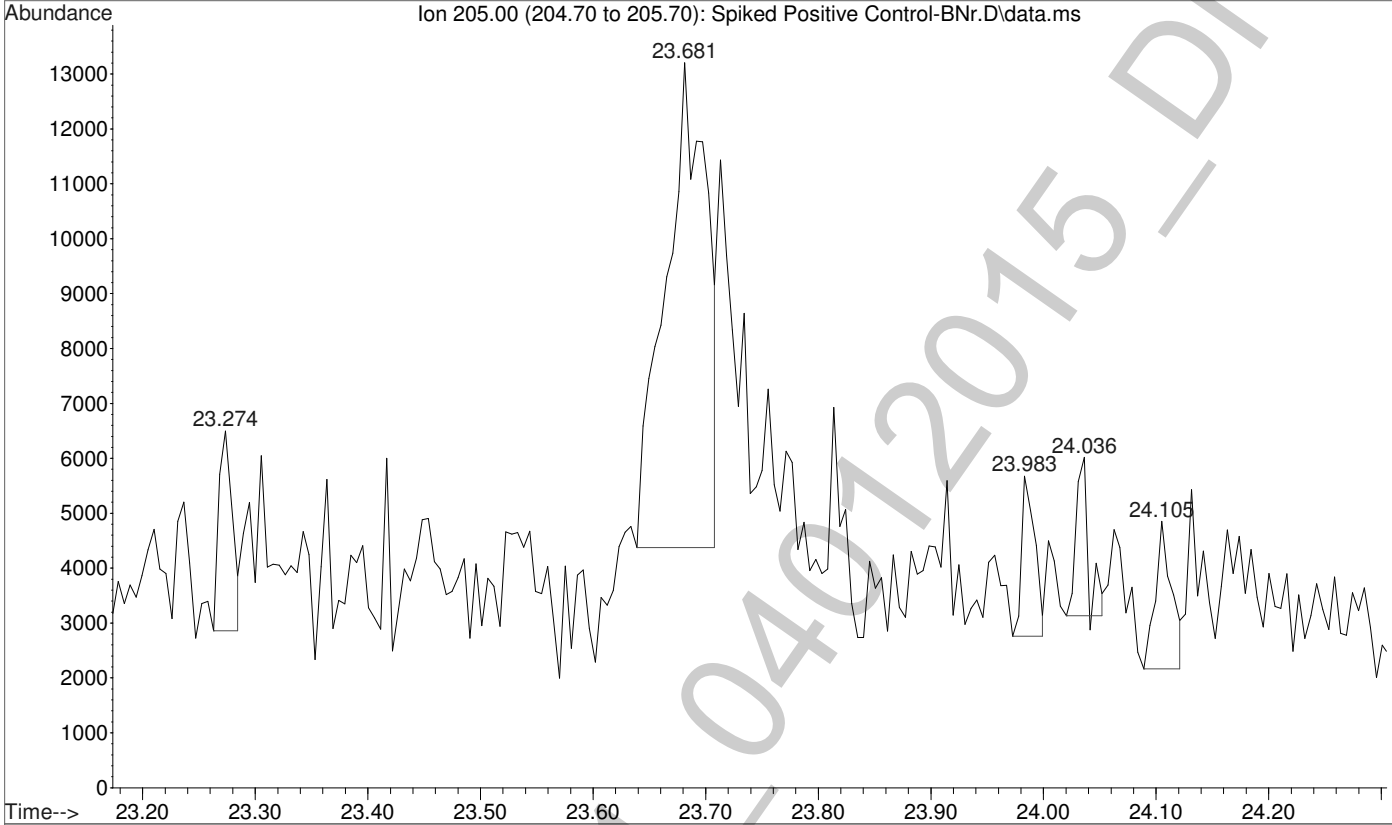

File :C:\gcms\1\data\Blood\040115BN\Reinjection Longer GC Method\p  
... rbLK2r.D  
Operator : 5LAB-C01\ISPuser  
Instrument : Major Mass Spec  
Acquired : 02 Apr 2015 02:00 using AcqMethod GBT092509-Delta EMV.M  
Sample Name: Solvent Blank  
Misc Info : Chloroform

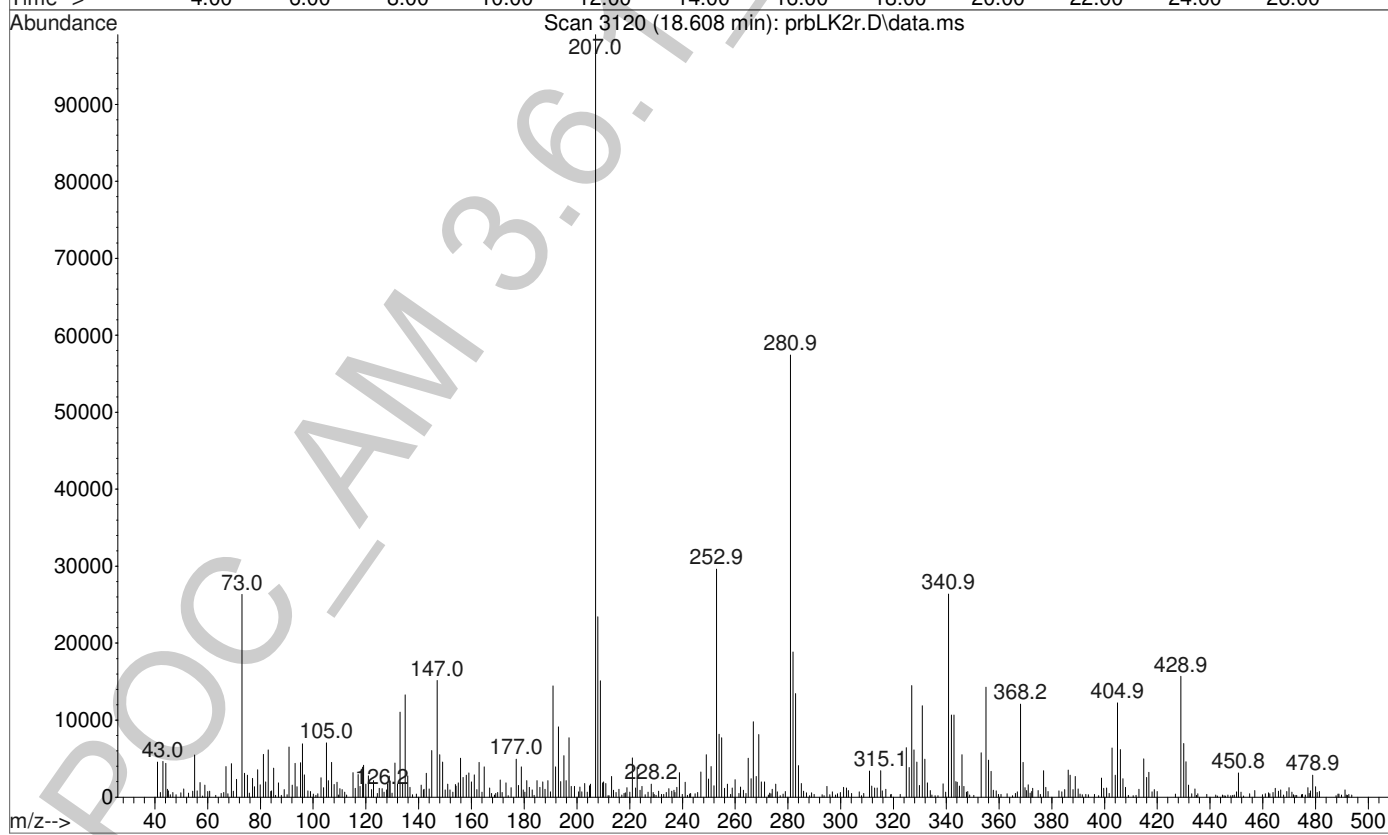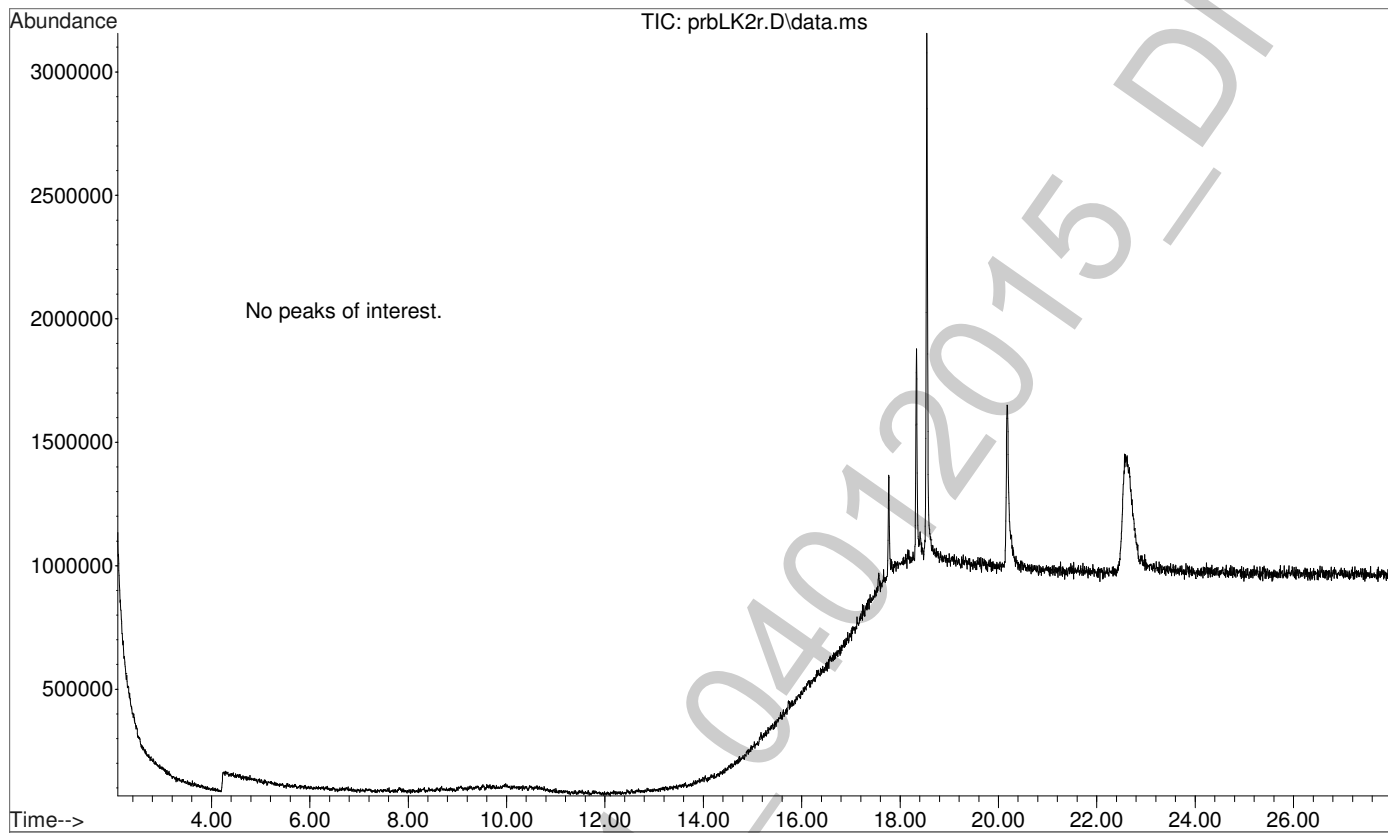

File :C:\gcms\1\data\Blood\040115BN\Reinjection Longer GC Method\P  
... OSTBLKr.D  
Operator : 5LAB-C01\ISPuser  
Instrument : Major Mass Spec  
Acquired : 04 Apr 2015 04:03 using AcqMethod BNSB120510.M  
Sample Name: BLK  
Misc Info : Chloroform

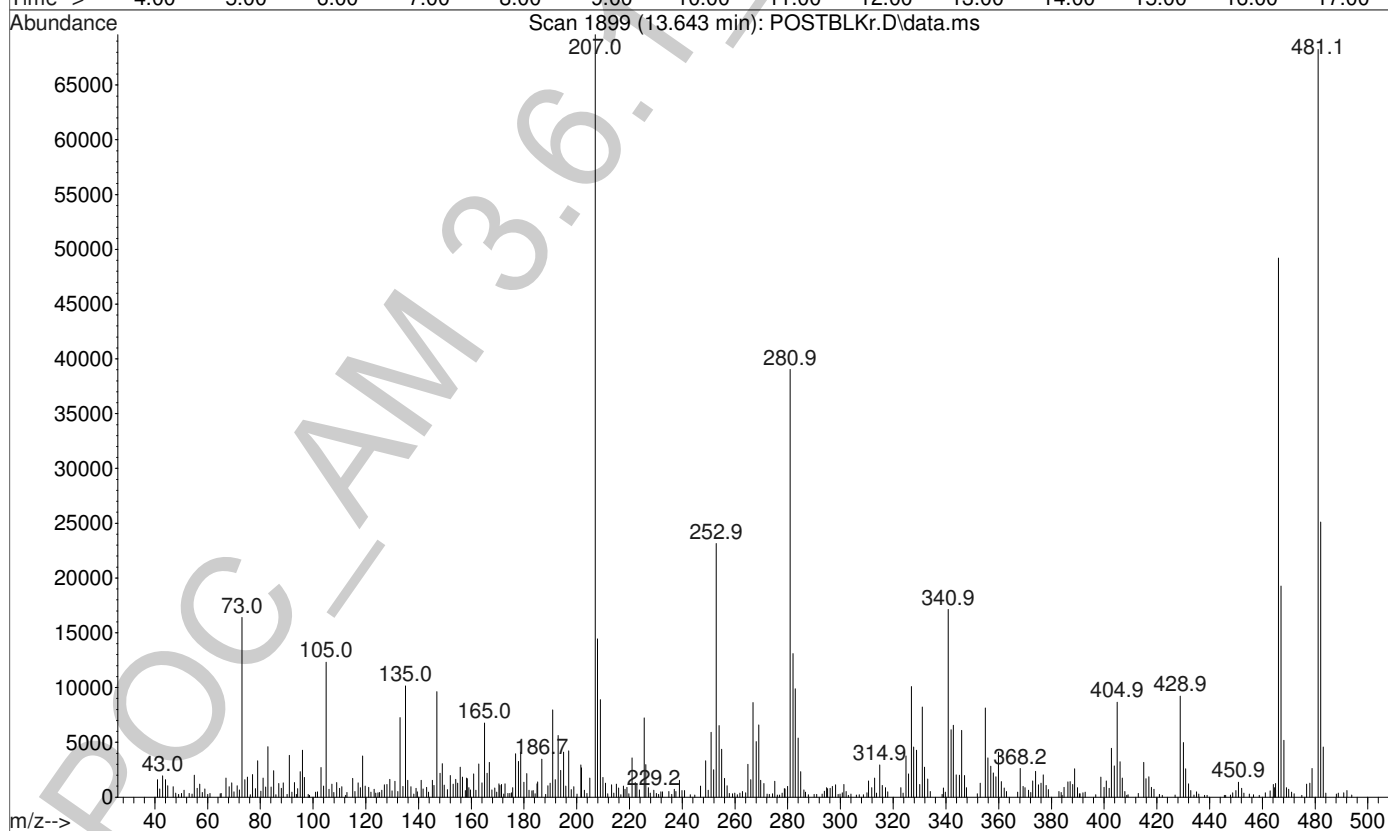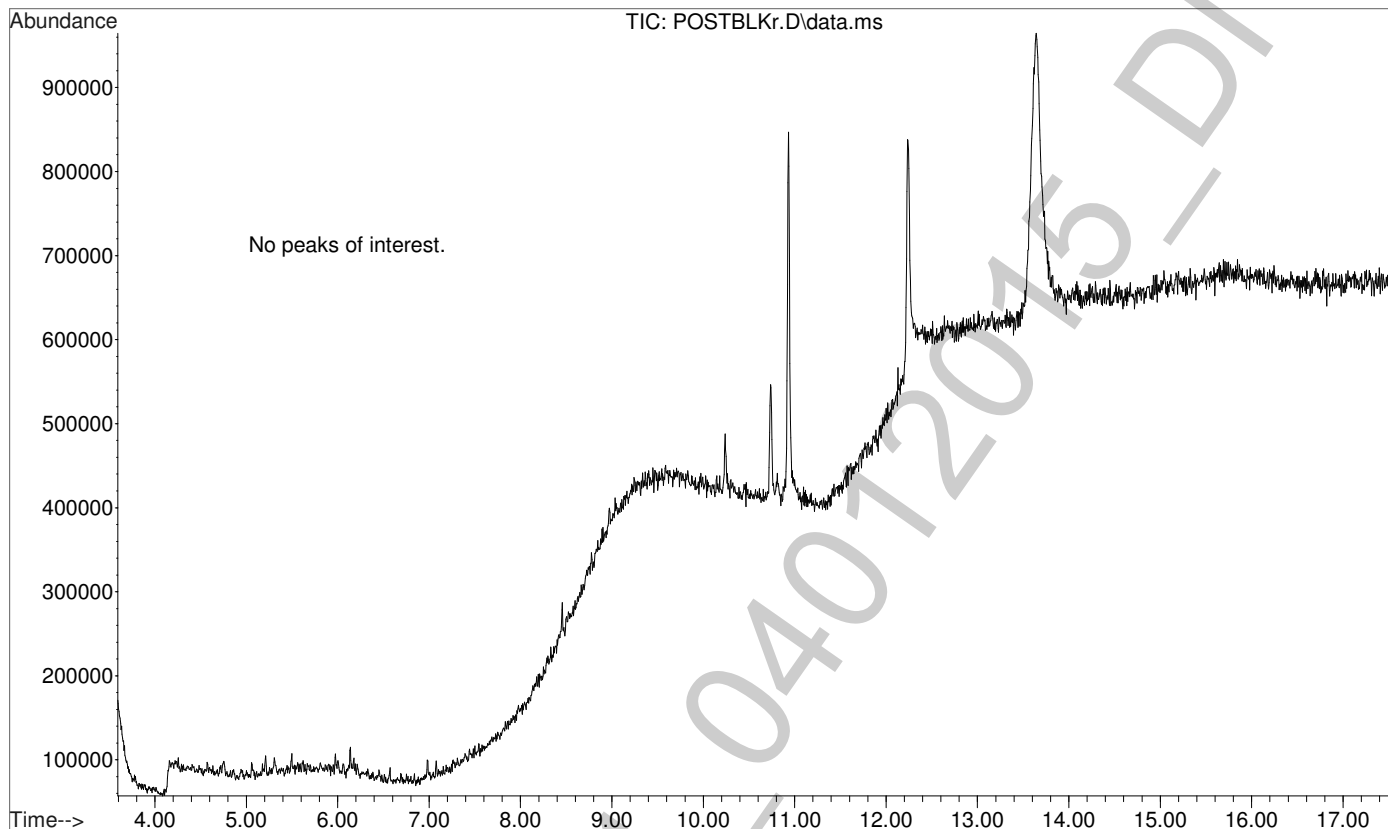

File :C:\gcms\1\data\Blood\040115BN\AFTER.D  
Operator : 5LAB-C01\ISPuser  
Acquired : 04 Apr 2015 04:25 using AcqMethod GBT092509-Delta EMV.M  
Instrument : Major Mass Spec  
Sample Name: BLK  
Misc Info : Chloroform  
Vial Number: 70

