

6/22/2015






Worklist: 747

| <u>LAB CASE</u> | <u>ITEM</u> | <u>TASK ID</u> | <u>DESCRIPTION</u> | |
|-----------------|-------------|----------------|----------------------------------|--|
| M2015-1481 | 1 | 33206 | 3.6.1 Blood base neutral confirr |  |
| M2015-1481 | 2 | 35563 | 3.6.1 Blood base neutral confirr |  |
| M2015-1510 | 1 | 33352 | 3.6.1 Blood base neutral confirr |  |
| M2015-1532 | 1 | 33407 | 3.6.1 Blood base neutral confirr |  |
| M2015-1618 | 1 | 33802 | 3.6.1 Blood base neutral confirr |  |
| M2015-1755 | 2 | 35065 | 3.6.1 Blood base neutral confirr |  |
| M2015-1827 | 6 | 35062 | 3.6.1 Blood base neutral confirr |  |
| M2015-1841 | 2 | 35045 | 3.6.1 Blood base neutral confirr |  |
| P2015-1243 | 1 | 34178 | 3.6.1 Blood base neutral confirr |  |
| P2015-1304 | 1 | 34876 | 3.6.1 Blood base neutral confirr |  |
| P2015-1308 | 1 | 34896 | 3.6.1 Blood base neutral confirr |  |
| P2015-1335 | 1 | 35059 | 3.6.1 Blood base neutral confirr |  |
| P2015-1336 | 1 | 35068 | 3.6.1 Blood base neutral confirr |  |
| P2015-1344 | 1 | 35122 | 3.6.1 Blood base neutral confirr |  |
| P2015-1346 | 1 | 35180 | 3.6.1 Blood base neutral confirr |  |
| P2015-1347 | 1 | 35183 | 3.6.1 Blood base neutral confirr |  |
| P2015-1348 | 1 | 35186 | 3.6.1 Blood base neutral confirr |  |
| P2015-1352 | 1 | 35202 | 3.6.1 Blood base neutral confirr |  |
| P2015-1383 | 1 | 35274 | 3.6.1 Blood base neutral confirr |  |
| P2015-1384 | 1 | 35277 | 3.6.1 Blood base neutral confirr |  |
| P2015-1389 | 1 | 35331 | 3.6.1 Blood base neutral confirr |  |
| P2015-1395 | 1 | 35464 | 3.6.1 Blood base neutral confirr |  |
| P2015-1396 | 1 | 35468 | 3.6.1 Blood base neutral confirr |  |

POC-AM3610612705

2

Worklist: 747

| <u>LAB_CASE</u> | <u>ITEM</u> | <u>TASK_ID</u> | <u>DESCRIPTION</u> | |
|-----------------|-------------|----------------|----------------------------------|--|
| P2015-1397 | 1 | 35484 | 3.6.1 Blood base neutral confirr |  |
| P2015-1398 | 1 | 35487 | 3.6.1 Blood base neutral confirr |  |
| P2015-1399 | 1 | 35491 | 3.6.1 Blood base neutral confirr |  |
| P2015-1404 | 1 | 35540 | 3.6.1 Blood base neutral confirr |  |
| P2015-1405 | 2 | 35567 | 3.6.1 Blood base neutral confirr |  |

POC_AM 3.6.1_06122015

6/12/15 eg

simulate_sequence.log
Simulate Run Sequence Fri Jun 12 12:53:18 2015

Instrument Name: Major Mass Spec
Sequence File: C:\Users\ISPuser\Desktop\Sequences\CS-BNSB.sequence.xml
Comment: MassHunter sequence
Operator: ISP\datastor
Data Path: D:\DATA\CDS\2015\New folder\
Method Path: D:\MassHunter\GCMS\1\methods\

| Line | Type | Vials | DataFile | Sample Name |
|---|--------|-------|-------------------------|---------------------------|
| Acquisition Method: BNSB120510.M | | | | |
| 1) | Sample | 100 | Prerun solvent Blank | Pre-run Solvent Blank |
| 2) | Sample | 1 | Negative Control-BN | Negative Control - ...068 |
| 3) | Sample | 2 | Spiked Positive Control | Positive Control |
| 4) | Sample | 99 | prBLK2 | Solvent Blank |
| Acquisition Method: GBT092509-Delta EMV.M | | | | |
| 5) | Sample | 100 | Prerun Solvent Blankr | Pre-run Solvent Blank |
| 6) | Sample | 1 | Negative Control-BNr | Negative Control - ...068 |
| 7) | Sample | 2 | Spiked Positive Control | Positive Control |
| 8) | Sample | 99 | prBLK2r | Solvent Blank |
| Acquisition Method: BNSB120510.M | | | | |
| 9) | Sample | 98 | M2015-1481-1-BNBLK | Lab No.: M2015-1481-1 |
| 10) | Sample | 3 | M2015-1481-1-BN | Lab No.: M2015-1481-1 |
| 11) | Sample | 97 | M2015-1481-2-BNBLK | Lab No.: M2015-1481-2 |
| 12) | Sample | 4 | M2015-1481-2-BN | Lab No.: M2015-1481-2 |
| 13) | Sample | 96 | M2015-1510-1-BNBLK | Lab No.: M2015-1510-1 |
| 14) | Sample | 5 | M2015-1510-1-BN | Lab No.: M2015-1510-1 |
| 15) | Sample | 95 | M2015-1532-1-BNBLK | Lab No.: M2015-1532-1 |
| 16) | Sample | 6 | M2015-1532-1-BN | Lab No.: M2015-1532-1 |
| 17) | Sample | 94 | M2015-1618-1-BNBLK | Lab No.: M2015-1618-1 |
| 18) | Sample | 7 | M2015-1618-1-BN | Lab No.: M2015-1618-1 |
| 19) | Sample | 93 | M2015-1755-2-BNBLK | Lab No.: M2015-1755-2 |
| 20) | Sample | 8 | M2015-1755-2-BN | Lab No.: M2015-1755-2 |
| 21) | Sample | 92 | M2015-1827-6-BNBLK | Lab No.: M2015-1827-6 |
| 22) | Sample | 9 | M2015-1827-6-BN | Lab No.: M2015-1827-6 |
| 23) | Sample | 91 | M2015-1841-2-BNBLK | Lab No.: M2015-1841-2 |
| 24) | Sample | 10 | M2015-1841-2-BN | Lab No.: M2015-1841-2 |
| Acquisition Method: GBT092509-Delta EMV.M | | | | |
| 25) | Sample | 98 | M2015-1481-1-BNBLKr | Lab No.: M2015-1481-1 |
| 26) | Sample | 3 | M2015-1481-1-BNr | Lab No.: M2015-1481-1 |
| 27) | Sample | 97 | M2015-1481-2-BNBLKr | Lab No.: M2015-1481-2 |
| 28) | Sample | 4 | M2015-1481-2-BNr | Lab No.: M2015-1481-2 |
| 29) | Sample | 96 | M2015-1510-1-BNBLKr | Lab No.: M2015-1510-1 |
| 30) | Sample | 5 | M2015-1510-1-BNr | Lab No.: M2015-1510-1 |
| 31) | Sample | 95 | M2015-1532-1-BNBLKr | Lab No.: M2015-1532-1 |
| 32) | Sample | 6 | M2015-1532-1-BNr | Lab No.: M2015-1532-1 |
| 33) | Sample | 94 | M2015-1618-1-BNBLKr | Lab No.: M2015-1618-1 |
| 34) | Sample | 7 | M2015-1618-1-BNr | Lab No.: M2015-1618-1 |
| 35) | Sample | 93 | M2015-1755-2-BNBLKr | Lab No.: M2015-1755-2 |
| 36) | Sample | 8 | M2015-1755-2-BNr | Lab No.: M2015-1755-2 |
| 37) | Sample | 92 | M2015-1827-6-BNBLKr | Lab No.: M2015-1827-6 |
| 38) | Sample | 9 | M2015-1827-6-BNr | Lab No.: M2015-1827-6 |
| 39) | Sample | 91 | M2015-1841-2-BNBLKr | Lab No.: M2015-1841-2 |
| 40) | Sample | 10 | M2015-1841-2-BNr | Lab No.: M2015-1841-2 |
| Acquisition Method: BNSB120510.M | | | | |
| 41) | Sample | 90 | P2015-1243-1-BNBLK | Lab No.: P2015-1243-1 |
| 42) | Sample | 11 | P2015-1243-1-BN | Lab No.: P2015-1243-1 |
| 43) | Sample | 89 | P2015-1304-1-BNBLK | Lab No.: P2015-1304-1 |
| 44) | Sample | 12 | P2015-1304-1-BN | Lab No.: P2015-1304-1 |
| 45) | Sample | 88 | P2015-1308-1-BNBLK | Lab No.: P2015-1308-1 |
| 46) | Sample | 13 | P2015-1308-1-BN | Lab No.: P2015-1308-1 |
| 47) | Sample | 87 | P2015-1335-1-BNBLK | Lab No.: P2015-1335-1 |
| 48) | Sample | 14 | P2015-1335-1-BN | Lab No.: P2015-1335-1 |

6/17/15 c
g

| simulate_sequence.log | | | |
|---|----|---------------------|-----------------------|
| 49) Sample | 86 | P2015-1336-1-BNBLK | Lab No.: P2015-1336-1 |
| 50) Sample | 15 | P2015-1336-1-BN | Lab No.: P2015-1336-1 |
| Acquisition Method: GBT092509-Delta EMV.M | | | |
| 51) Sample | 90 | P2015-1243-1-BNBLKr | Lab No.: P2015-1243-1 |
| 52) Sample | 11 | P2015-1243-1-BNr | Lab No.: P2015-1243-1 |
| 53) Sample | 89 | P2015-1304-1-BNBLKr | Lab No.: P2015-1304-1 |
| 54) Sample | 12 | P2015-1304-1-BNr | Lab No.: P2015-1304-1 |
| 55) Sample | 88 | P2015-1308-1-BNBLKr | Lab No.: P2015-1308-1 |
| 56) Sample | 13 | P2015-1308-1-BNr | Lab No.: P2015-1308-1 |
| 57) Sample | 87 | P2015-1335-1-BNBLKr | Lab No.: P2015-1335-1 |
| 58) Sample | 14 | P2015-1335-1-BNr | Lab No.: P2015-1335-1 |
| 59) Sample | 86 | P2015-1336-1-BNBLKr | Lab No.: P2015-1336-1 |
| 60) Sample | 15 | P2015-1336-1-BNr | Lab No.: P2015-1336-1 |
| Acquisition Method: BNSB120510.M | | | |
| 61) Sample | 85 | P2015-1344-1-BNBLK | Lab No.: P2015-1344-1 |
| 62) Sample | 16 | P2015-1344-1-BN | Lab No.: P2015-1344-1 |
| 63) Sample | 84 | P2015-1346-1-BNBLK | Lab No.: P2015-1346-1 |
| 64) Sample | 17 | P2015-1346-1-BN | Lab No.: P2015-1346-1 |
| 65) Sample | 83 | P2015-1347-1-BNBLK | Lab No.: P2015-1347-1 |
| 66) Sample | 18 | P2015-1347-1-BN | Lab No.: P2015-1347-1 |
| 67) Sample | 82 | P2015-1348-1-BNBLK | Lab No.: P2015-1348-1 |
| 68) Sample | 19 | P2015-1348-1-BN | Lab No.: P2015-1348-1 |
| 69) Sample | 81 | P2015-1352-1-BNBLK | Lab No.: P2015-1352-1 |
| 70) Sample | 20 | P2015-1352-1-BN | Lab No.: P2015-1352-1 |
| Acquisition Method: GBT092509-Delta EMV.M | | | |
| 71) Sample | 85 | P2015-1344-1-BNBLKr | Lab No.: P2015-1344-1 |
| 72) Sample | 16 | P2015-1344-1-BNr | Lab No.: P2015-1344-1 |
| 73) Sample | 84 | P2015-1346-1-BNBLKr | Lab No.: P2015-1346-1 |
| 74) Sample | 17 | P2015-1346-1-BNr | Lab No.: P2015-1346-1 |
| 75) Sample | 83 | P2015-1347-1-BNBLKr | Lab No.: P2015-1347-1 |
| 76) Sample | 18 | P2015-1347-1-BNr | Lab No.: P2015-1347-1 |
| 77) Sample | 82 | P2015-1348-1-BNBLKr | Lab No.: P2015-1348-1 |
| 78) Sample | 19 | P2015-1348-1-BNr | Lab No.: P2015-1348-1 |
| 79) Sample | 81 | P2015-1352-1-BNBLKr | Lab No.: P2015-1352-1 |
| 80) Sample | 20 | P2015-1352-1-BNr | Lab No.: P2015-1352-1 |
| Acquisition Method: BNSB120510.M | | | |
| 81) Sample | 80 | P2015-1383-1-BNBLK | Lab No.: P2015-1383-1 |
| 82) Sample | 21 | P2015-1383-1-BN | Lab No.: P2015-1383-1 |
| 83) Sample | 79 | P2015-1384-1-BNBLK | Lab No.: P2015-1384-1 |
| 84) Sample | 22 | P2015-1384-1-BN | Lab No.: P2015-1384-1 |
| 85) Sample | 78 | P2015-1389-1-BNBLK | Lab No.: P2015-1389-1 |
| 86) Sample | 23 | P2015-1389-1-BN | Lab No.: P2015-1389-1 |
| 87) Sample | 77 | P2015-1395-1-BNBLK | Lab No.: P2015-1395-1 |
| 88) Sample | 24 | P2015-1395-1-BN | Lab No.: P2015-1395-1 |
| 89) Sample | 76 | P2015-1396-1-BNBLK | Lab No.: P2015-1396-1 |
| 90) Sample | 25 | P2015-1396-1-BN | Lab No.: P2015-1396-1 |
| Acquisition Method: GBT092509-Delta EMV.M | | | |
| 91) Sample | 80 | P2015-1383-1-BNBLKr | Lab No.: P2015-1383-1 |
| 92) Sample | 21 | P2015-1383-1-BNr | Lab No.: P2015-1383-1 |
| 93) Sample | 79 | P2015-1384-1-BNBLKr | Lab No.: P2015-1384-1 |
| 94) Sample | 22 | P2015-1384-1-BNr | Lab No.: P2015-1384-1 |
| 95) Sample | 78 | P2015-1389-1-BNBLKr | Lab No.: P2015-1389-1 |
| 96) Sample | 23 | P2015-1389-1-BNr | Lab No.: P2015-1389-1 |
| 97) Sample | 77 | P2015-1395-1-BNBLKr | Lab No.: P2015-1395-1 |
| 98) Sample | 24 | P2015-1395-1-BNr | Lab No.: P2015-1395-1 |
| 99) Sample | 76 | P2015-1396-1-BNBLKr | Lab No.: P2015-1396-1 |
| 100) Sample | 25 | P2015-1396-1-BNr | Lab No.: P2015-1396-1 |
| Acquisition Method: BNSB120510.M | | | |
| 101) Sample | 75 | P2015-1397-1-BNBLK | Lab No.: P2015-1397-1 |
| 102) Sample | 26 | P2015-1397-1-BN | Lab No.: P2015-1397-1 |
| Acquisition Method: GBT092509-Delta EMV.M | | | |

6/17/15 c
e

```
simulate_sequence.log
103) Sample      75      P2015-1397-1-BNBLKr  Lab No.: P2015-1397-1
104) Sample      26      P2015-1397-1-BNr    Lab No.: P2015-1397-1

Acquisition Method: BNSB120510.M
105) Sample      74      P2015-1398-1-BNBLK  Lab No.: P2015-1398-1
106) Sample      27      P2015-1398-1-BN     Lab No.: P2015-1398-1

Acquisition Method: GBT092509-Delta EMV.M
107) Sample      74      P2015-1398-1-BNBLKr Lab No.: P2015-1398-1
108) Sample      27      P2015-1398-1-BNr    Lab No.: P2015-1398-1

Acquisition Method: BNSB120510.M
109) Sample      73      P2015-1399-1-BNBLK  Lab No.: P2015-1399-1
110) Sample      28      P2015-1399-1-BN     Lab No.: P2015-1399-1
111) Sample      72      P2015-1404-1-BNBLK  Lab No.: P2015-1404-1
112) Sample      29      P2015-1404-1-BN     Lab No.: P2015-1404-1
113) Sample      71      P2015-1405-2-BNBLK  Lab No.: P2015-1405-2
114) Sample      30      P2015-1405-2-BN     Lab No.: P2015-1405-2

Acquisition Method: GBT092509-Delta EMV.M
115) Sample      73      P2015-1399-1-BNBLKr Lab No.: P2015-1399-1
116) Sample      28      P2015-1399-1-BNr    Lab No.: P2015-1399-1
117) Sample      72      P2015-1404-1-BNBLKr Lab No.: P2015-1404-1
118) Sample      29      P2015-1404-1-BNr    Lab No.: P2015-1404-1
119) Sample      71      P2015-1405-2-BNBLKr Lab No.: P2015-1405-2
120) Sample      30      P2015-1405-2-BNr    Lab No.: P2015-1405-2

Acquisition Method: BNSB120510.M
121) Sample      70      POSTBLK              BLK

Acquisition Method: GBT092509-Delta EMV.M
122) Sample      69      AFTER                BLK
megabytes Needed: 2605 Space on drive D: 292468
Sequence Verification Done!
```

POC_AM 3.6.1

2

Analytical Method 3.6.1 & 3.6.7 QA Check List

Run Start Date: 06/12/15

Analyst: CS

(Short GC/MS temperature program)

Positive Control Compound List

- Methamphetamine
- Nicotine
- Meperidine
- Caffeine
- Diphenhydramine
- Lidocaine
- PCP
- Methadone
- Amitriptyline
- Codeine
- Trazodone


Internal Standards

- Benzphetamine
- Papaverine

Optional back extraction **not** performed.
Reconstituted in MeOH.



2

File :I:\Celena\061215\Negative Control-BN.D
Operator : ISP\datastor
Acquired : 12 Jun 2015 13:29 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1
Vial Number: 1

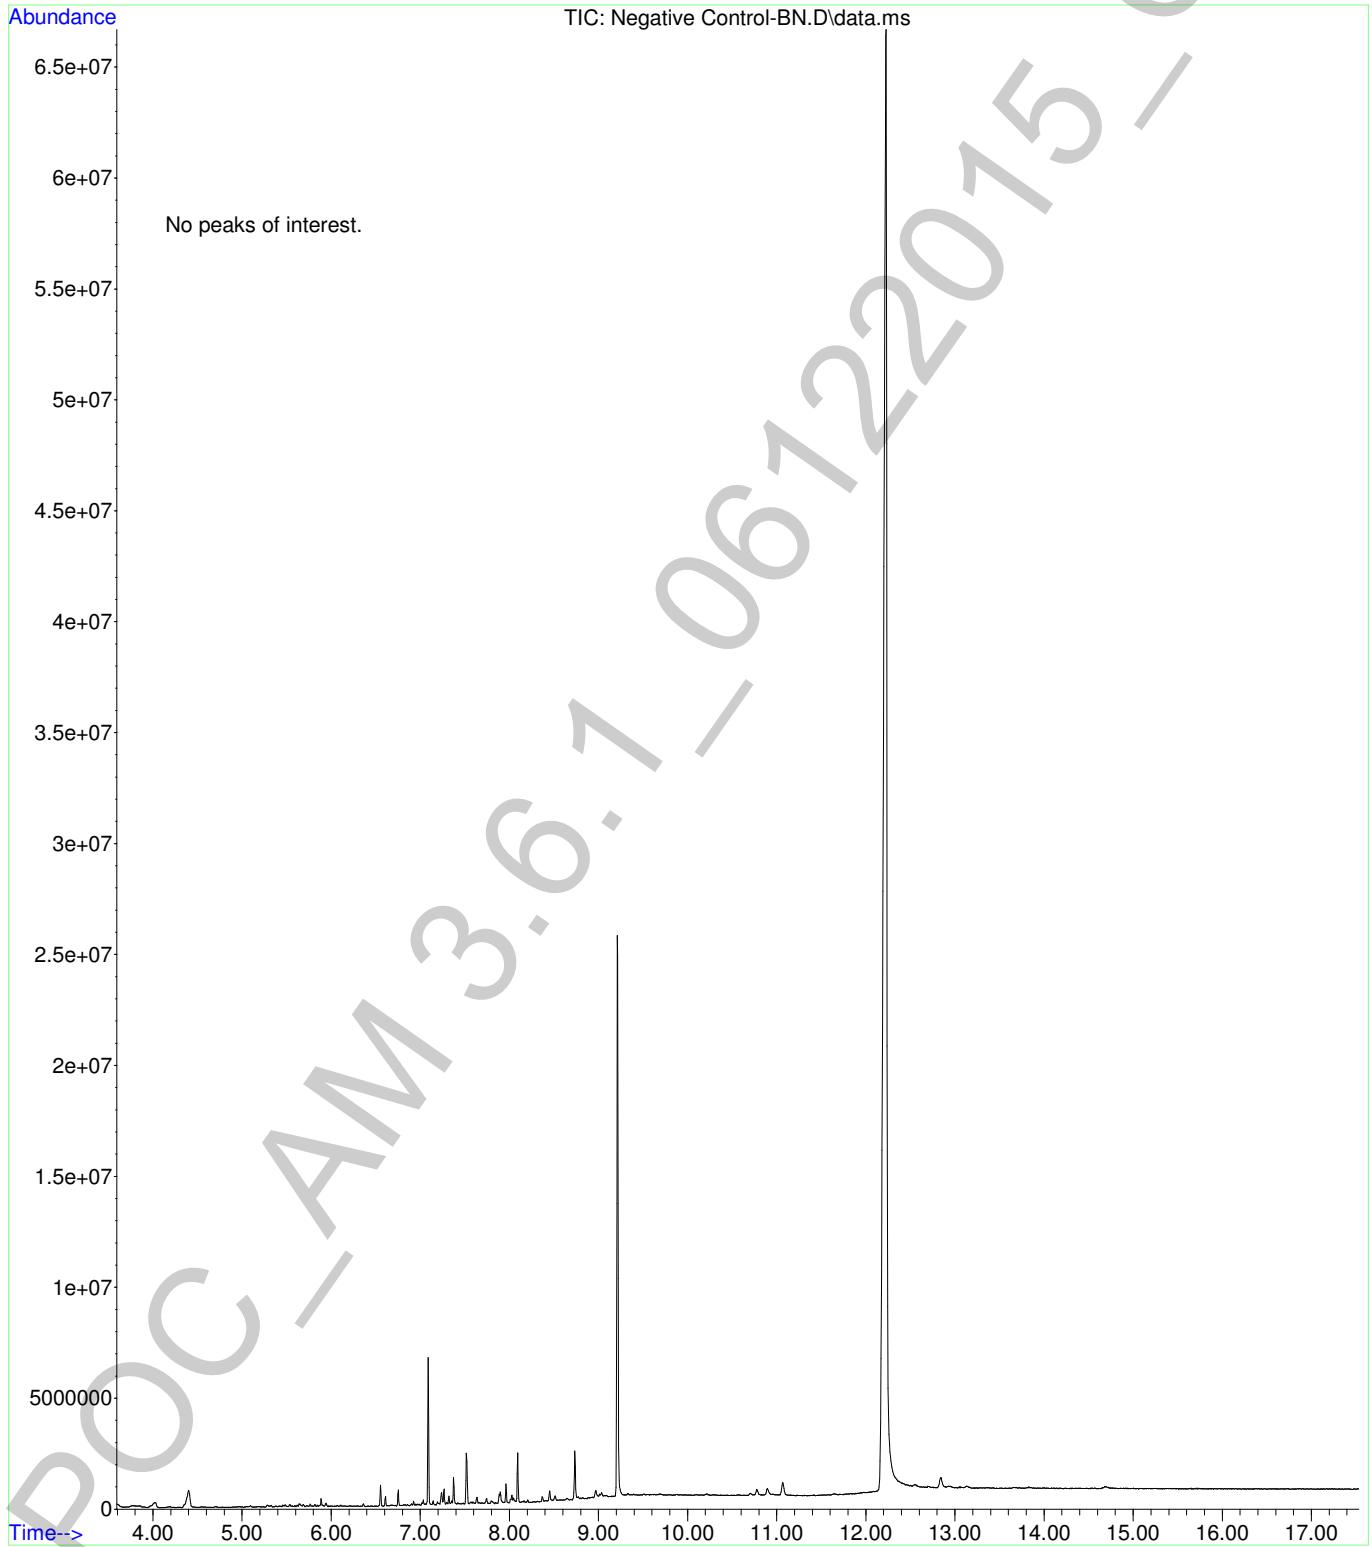



2

File : I:\Celena\061215\Negative Control-BN.D
Operator : ISP\datastor
Acquired : 12 Jun 2015 13:29 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1
Vial Number: 1

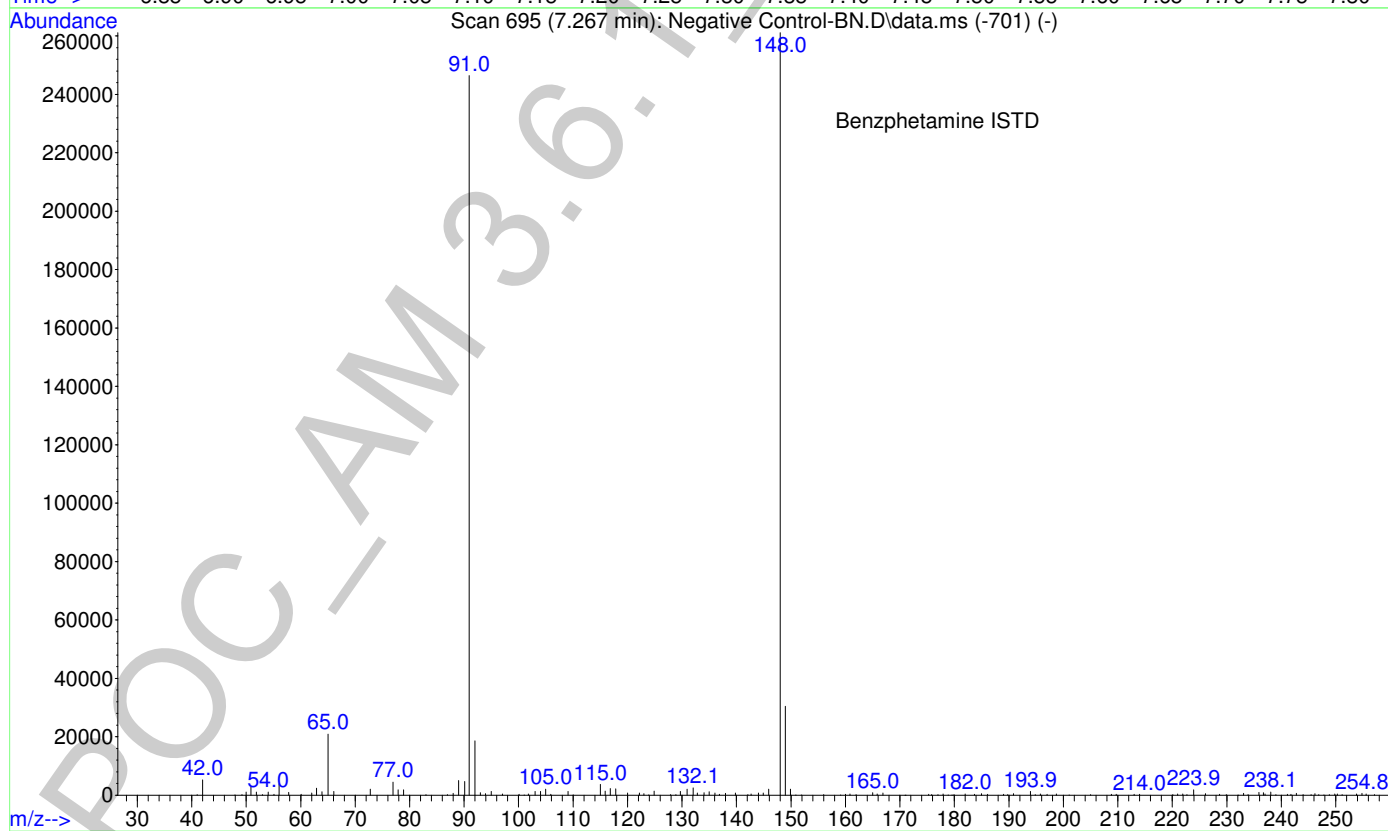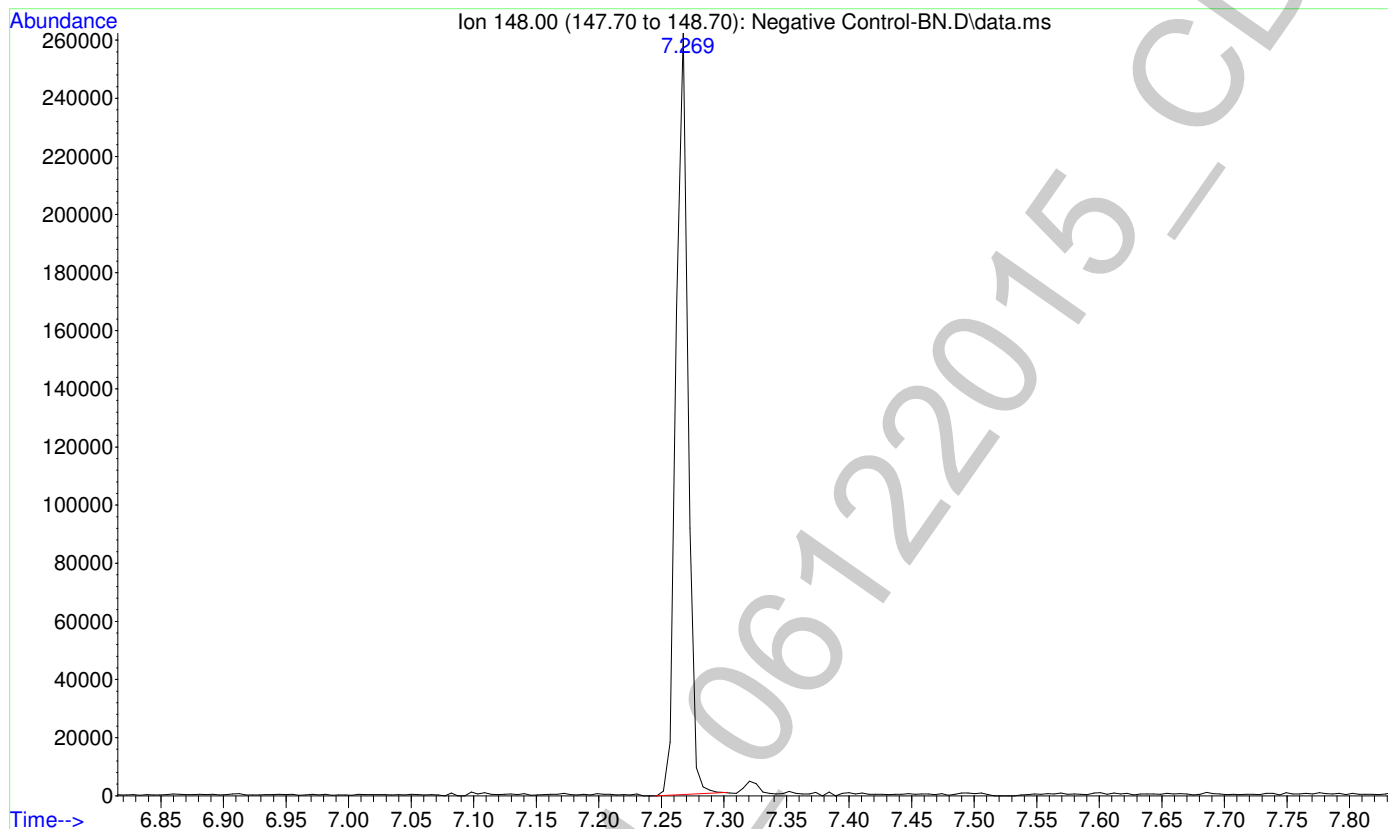


File : I:\Celena\061215\Negative Control-BN.D
Operator : ISP\datastor
Acquired : 12 Jun 2015 13:29 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1
Vial Number: 1

6

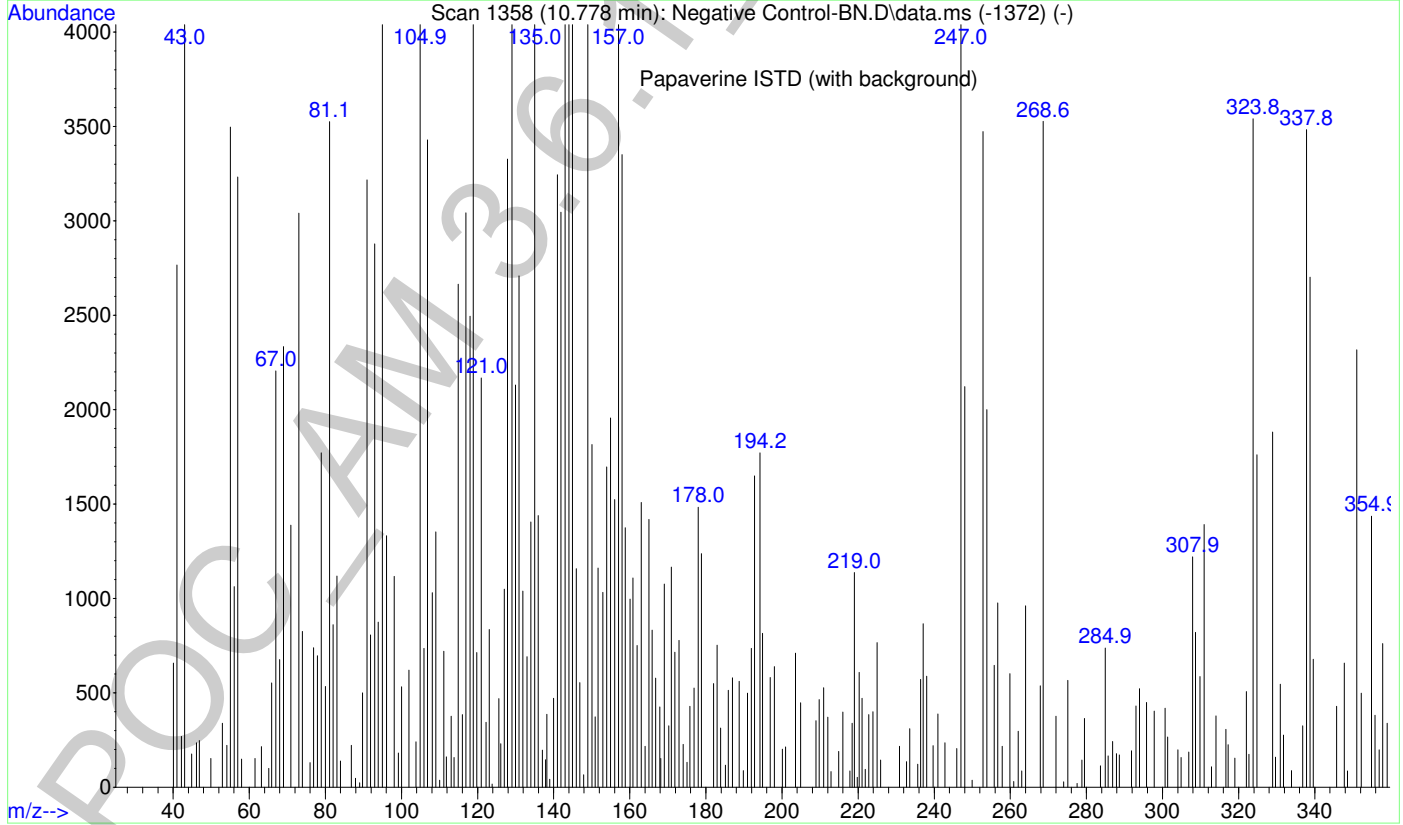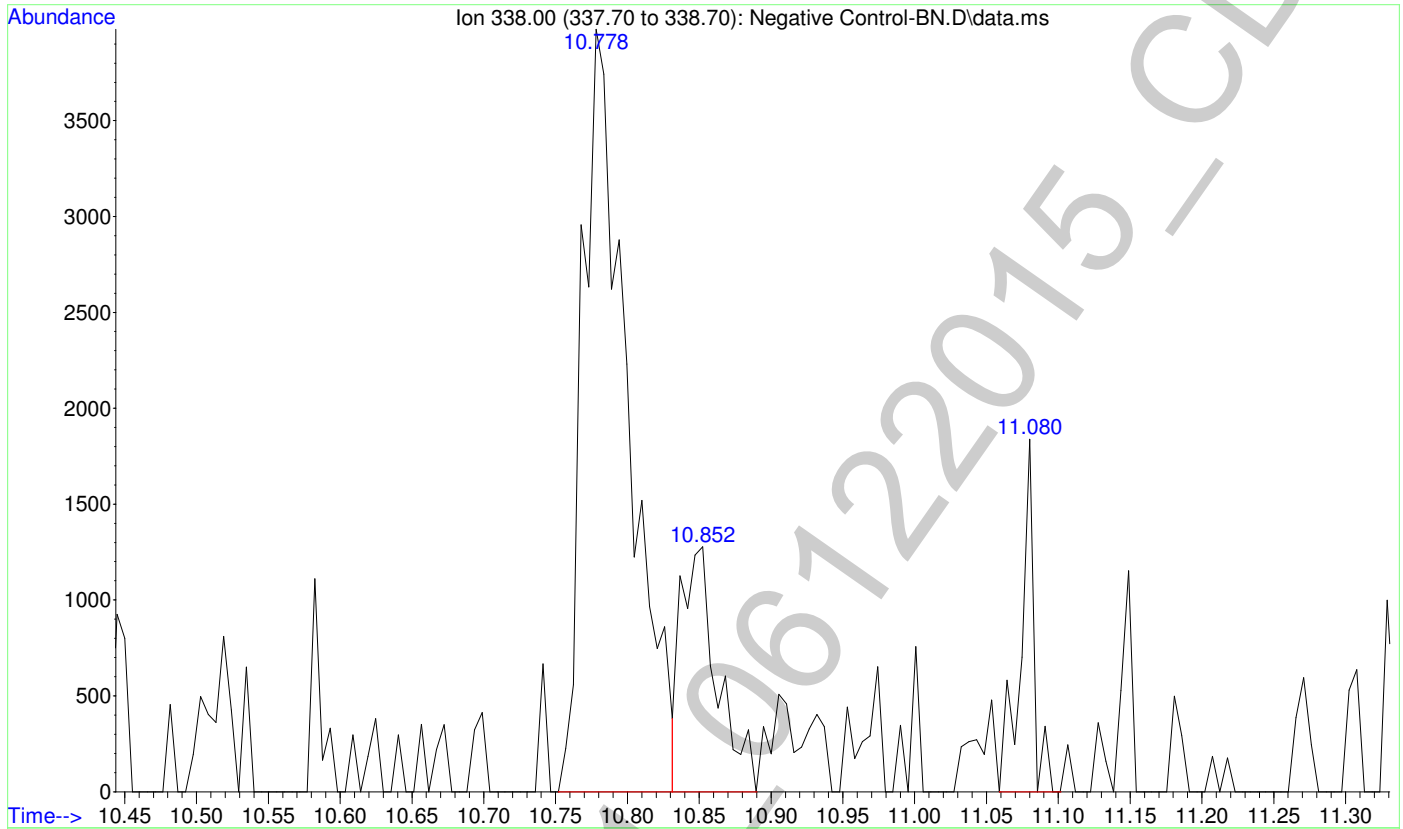



2

File :C:\MyFiles\cshrum\Desktop\Data\061215\Spiked Positive Contro
... 1-BN.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 12 Jun 2015 13:52 using AcqMethod BNSB120510.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

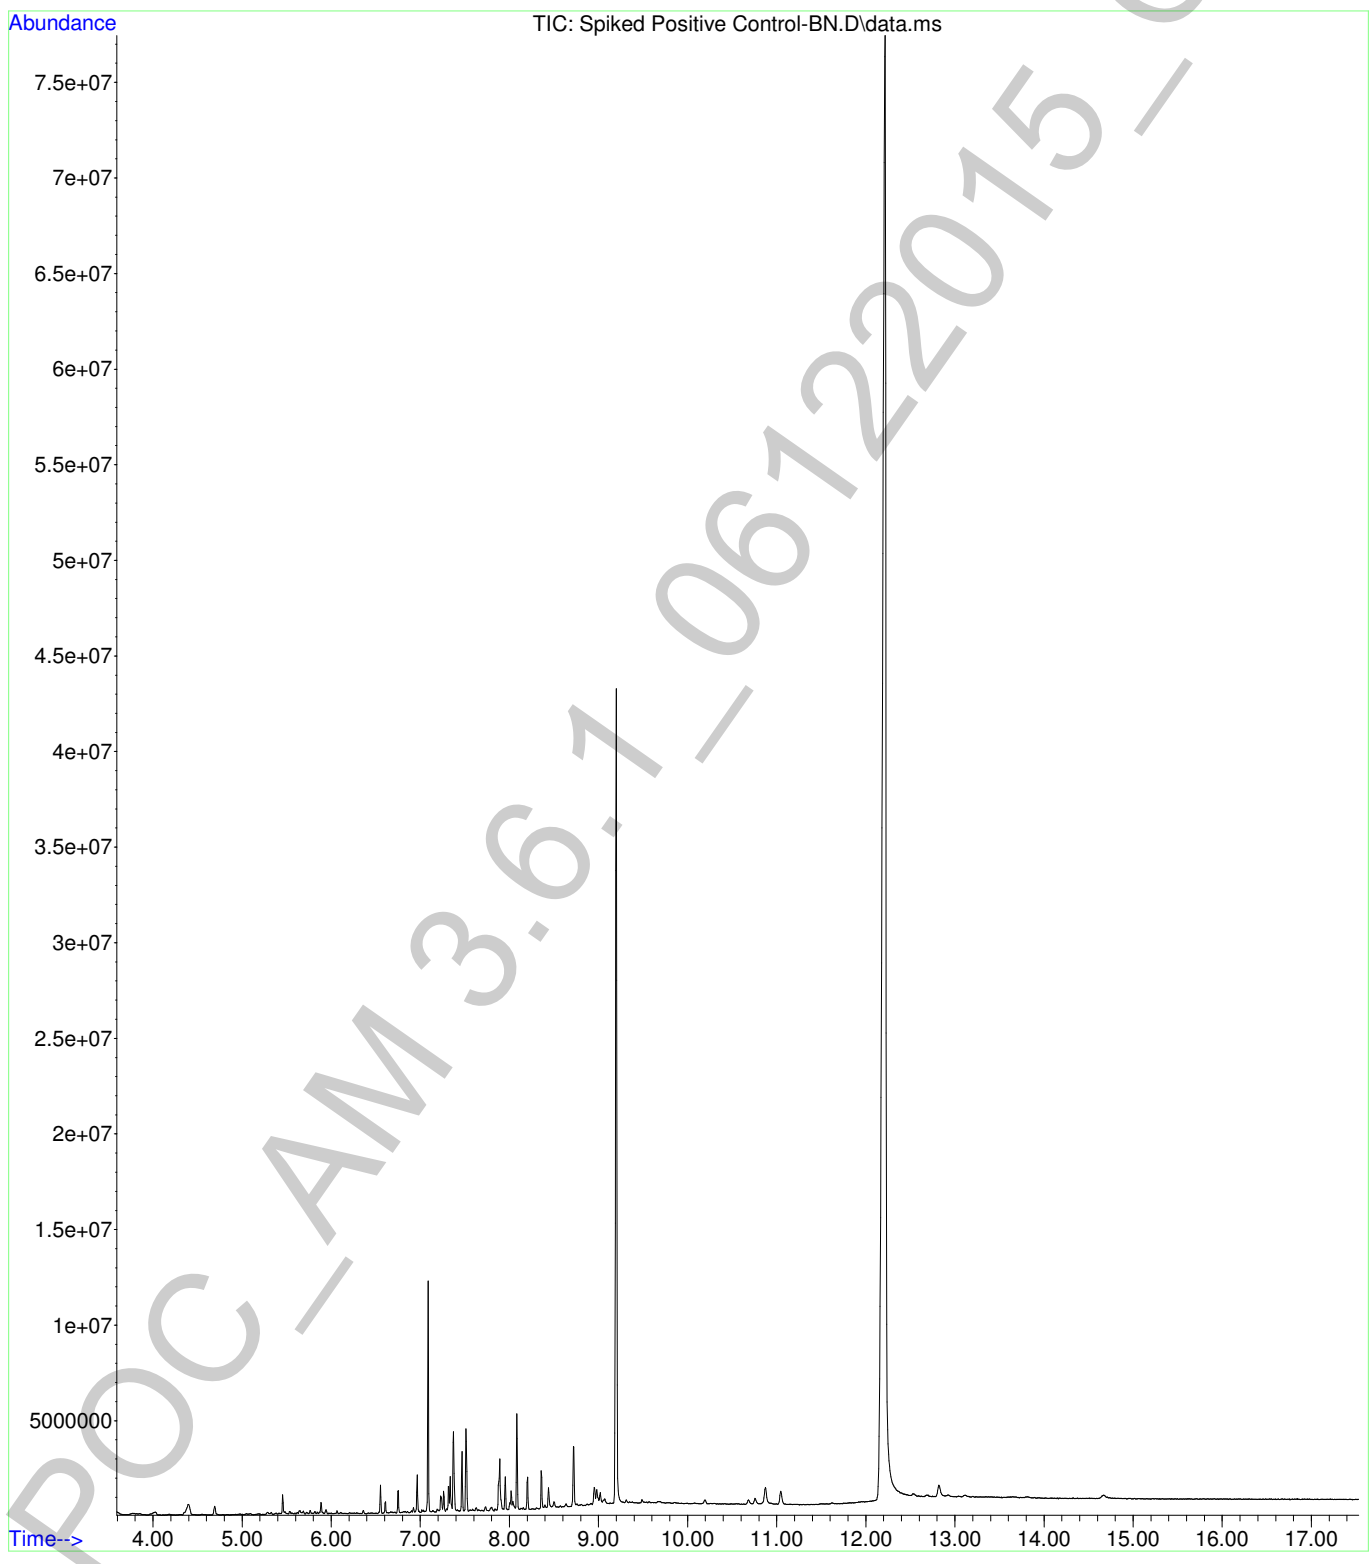



2

File : I:\Celena\061215\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 12 Jun 2015 13:52 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

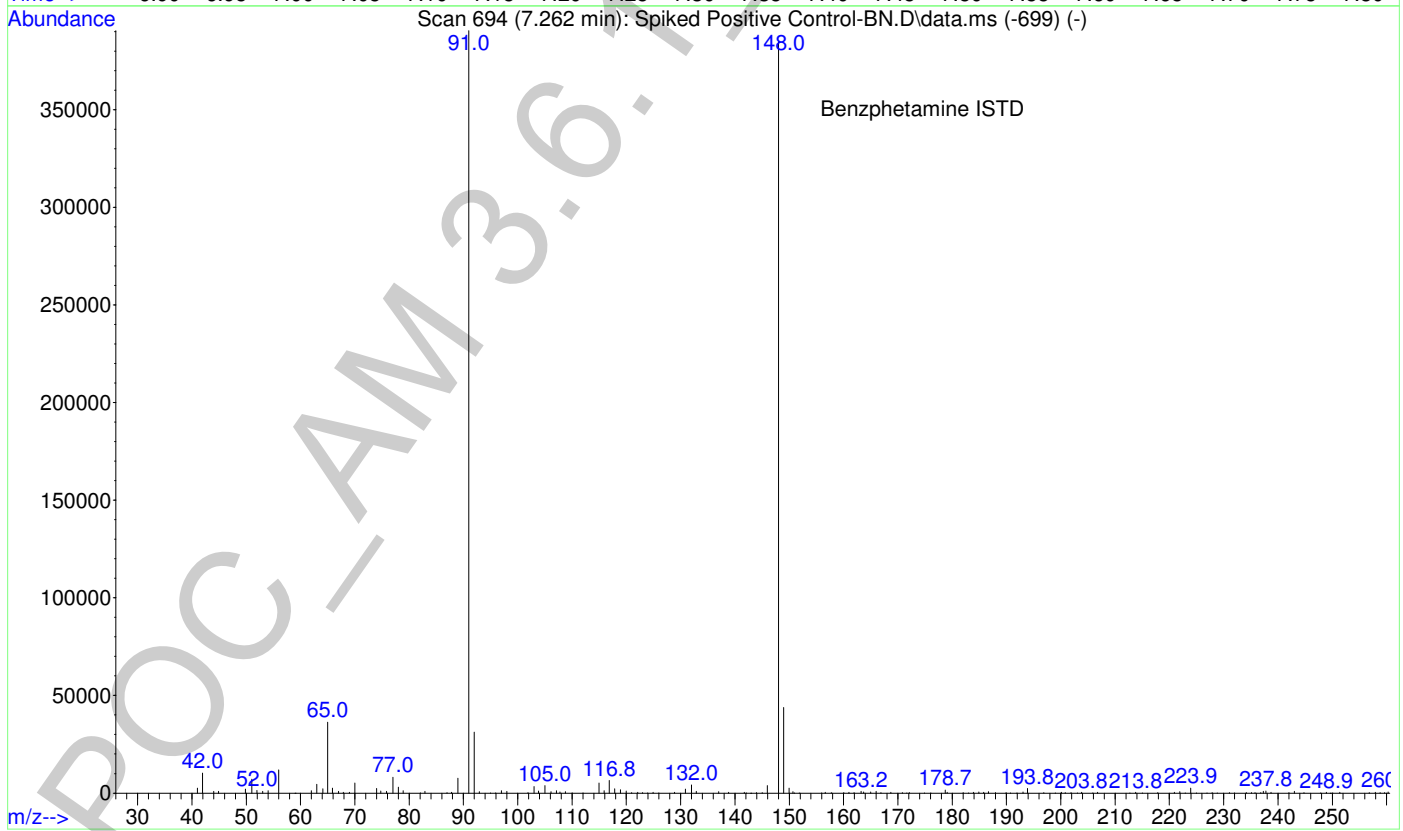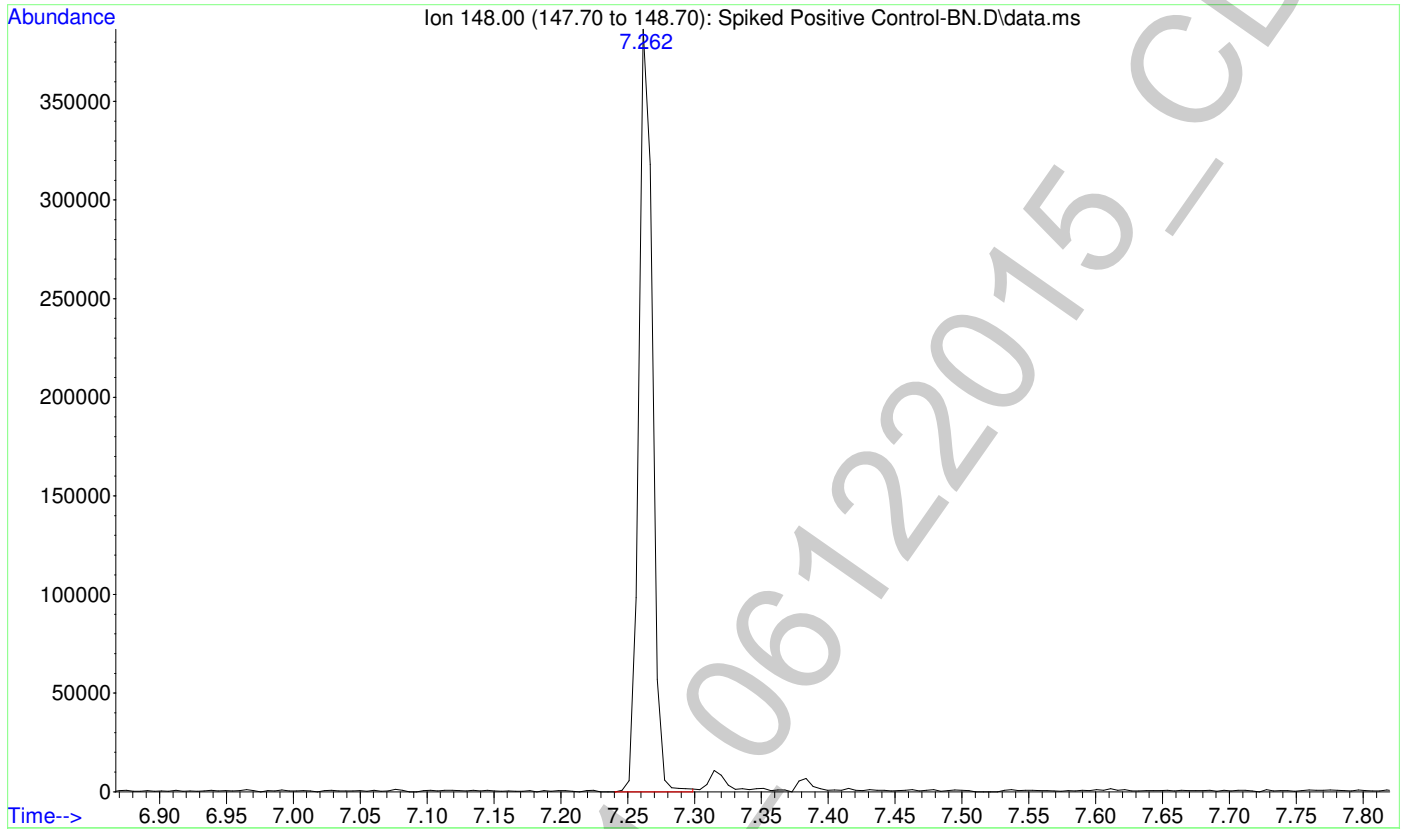



File : I:\Celena\061215\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 12 Jun 2015 13:52 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

2

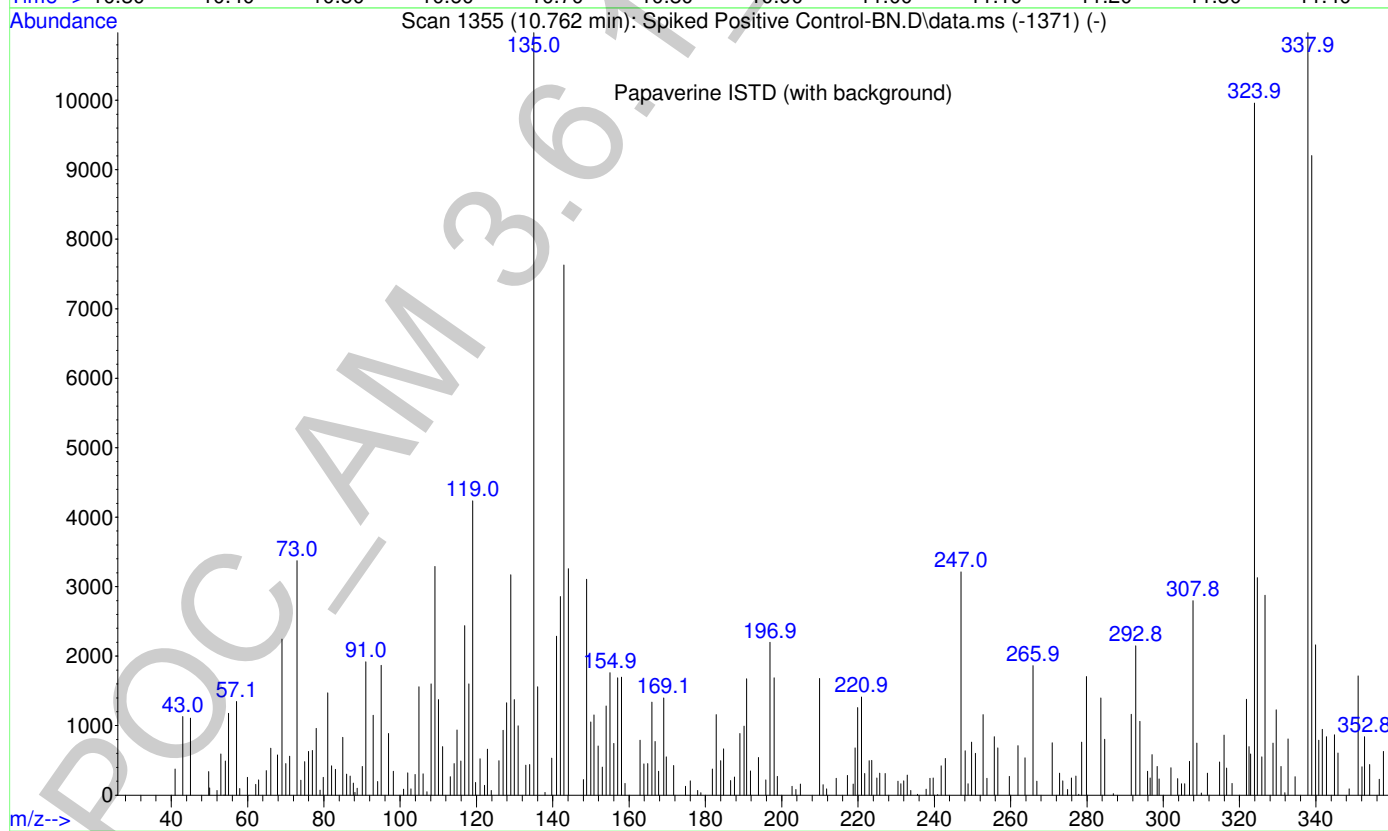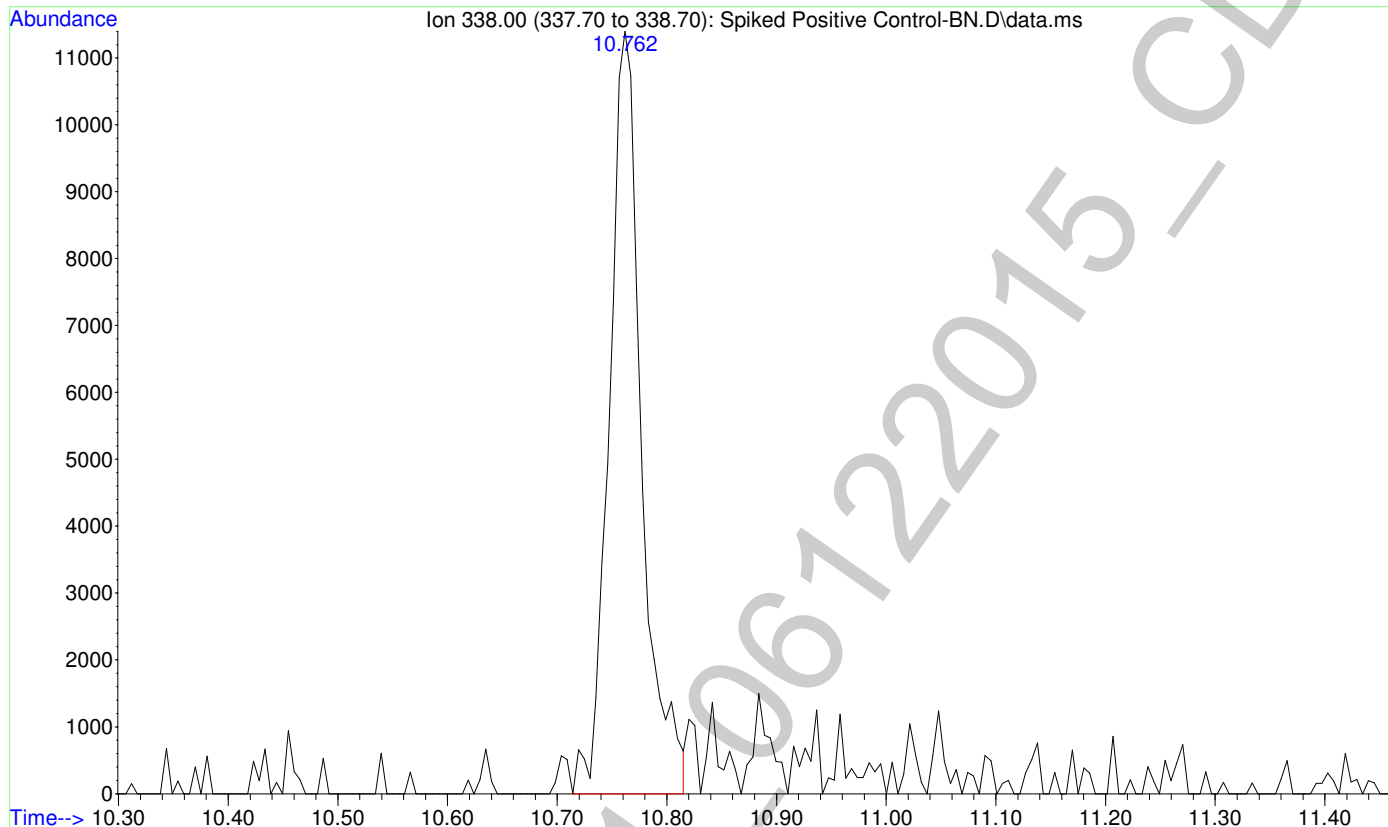



File : I:\Celena\061215\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 12 Jun 2015 13:52 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

2

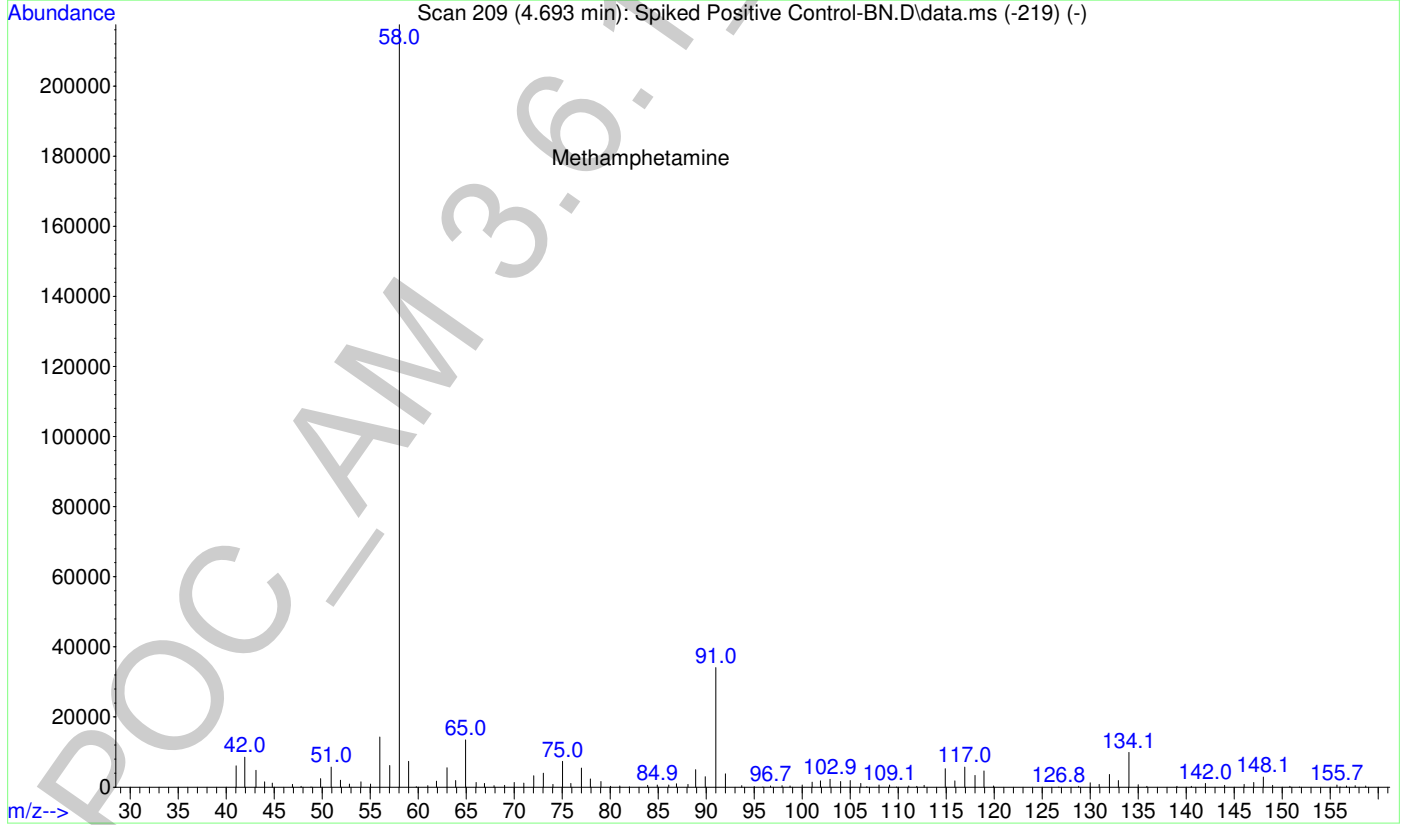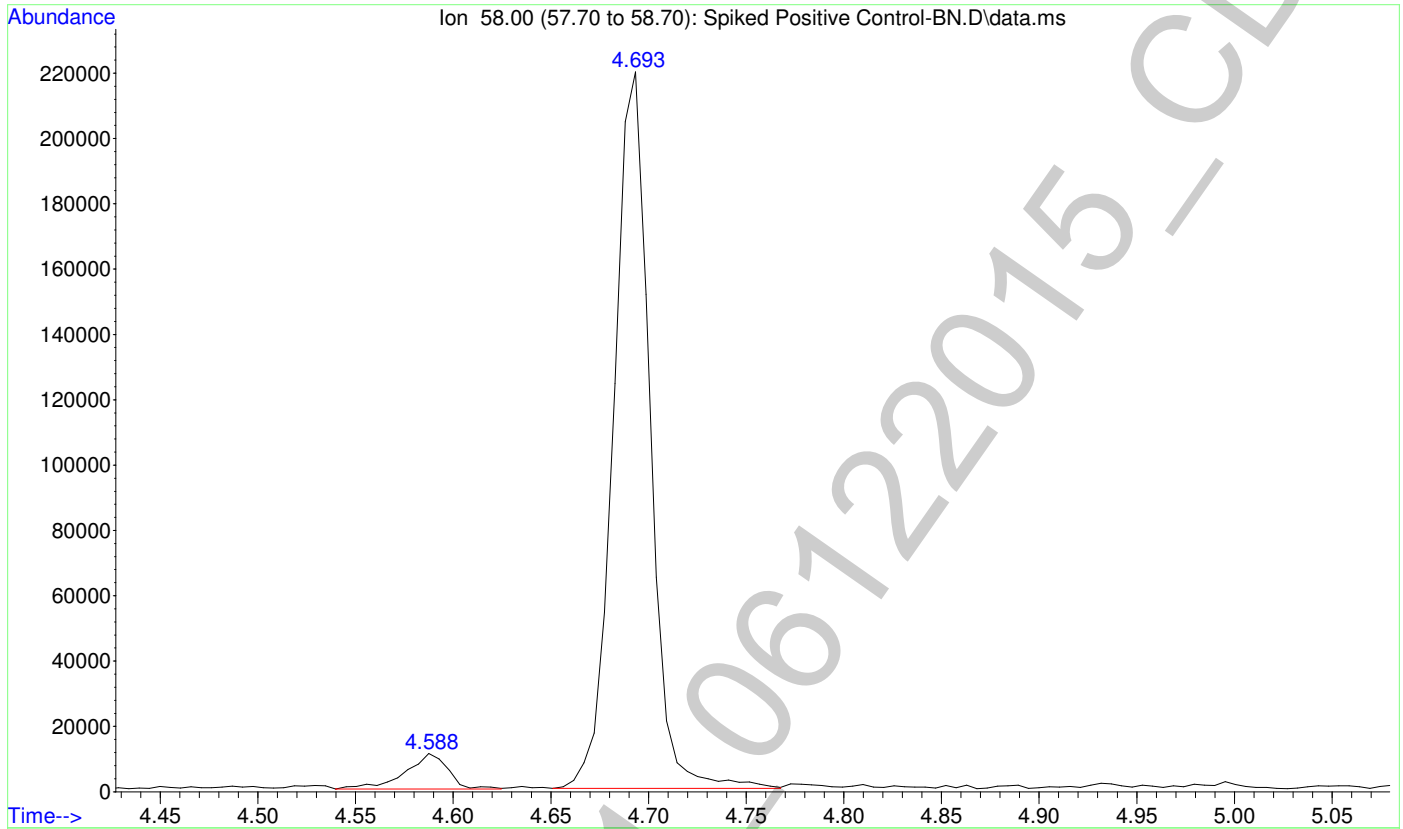



2

File : I:\Celena\061215\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 12 Jun 2015 13:52 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

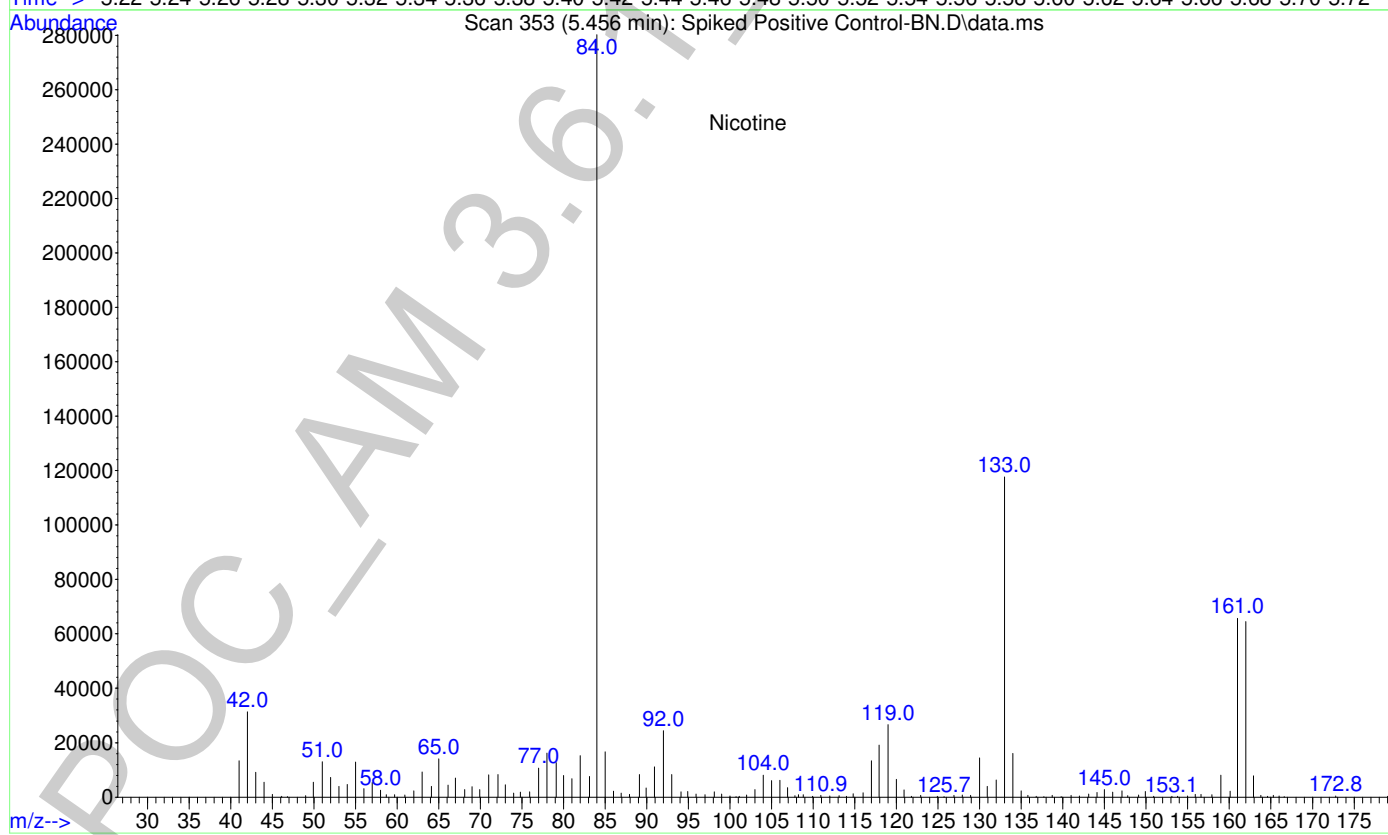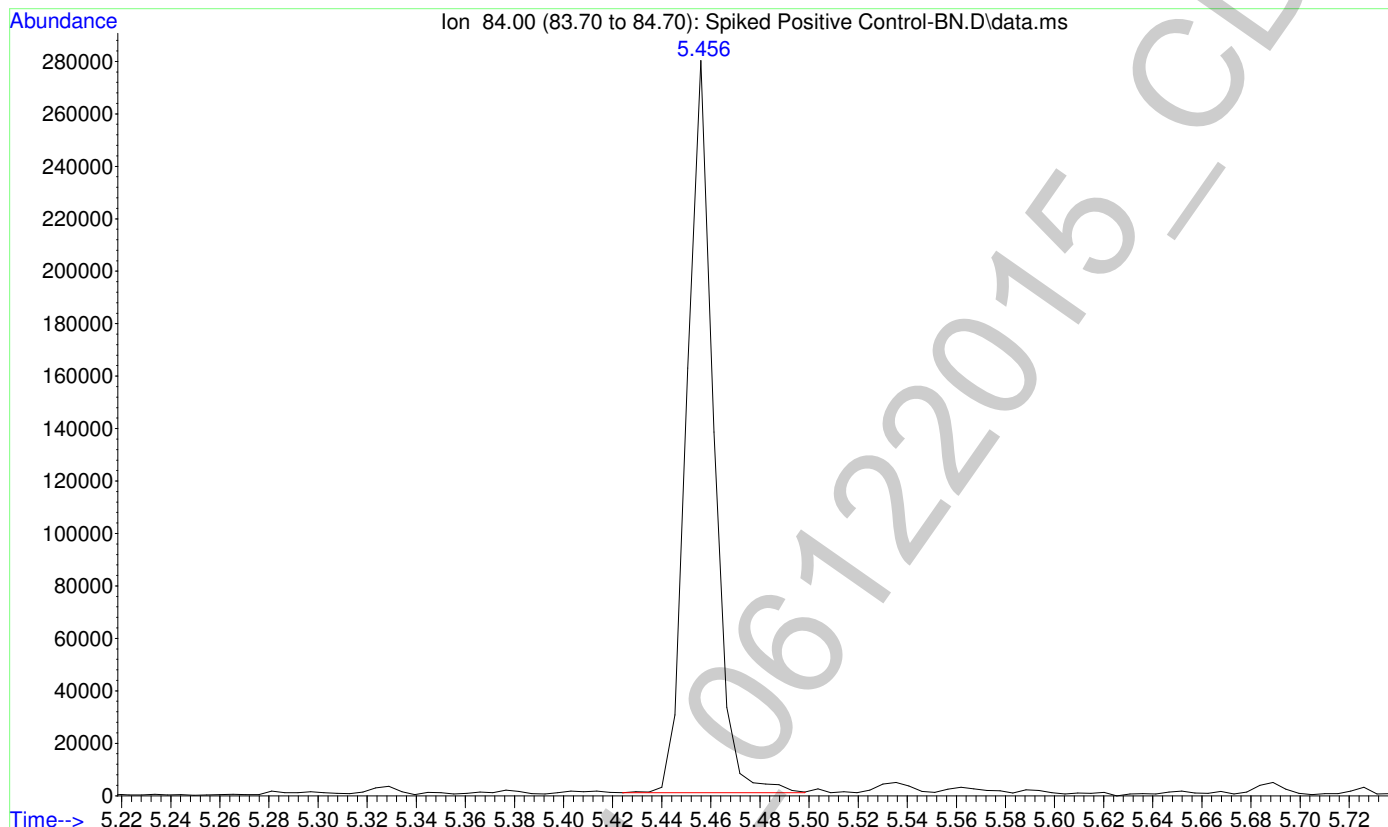



2

File : I:\Celena\061215\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 12 Jun 2015 13:52 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

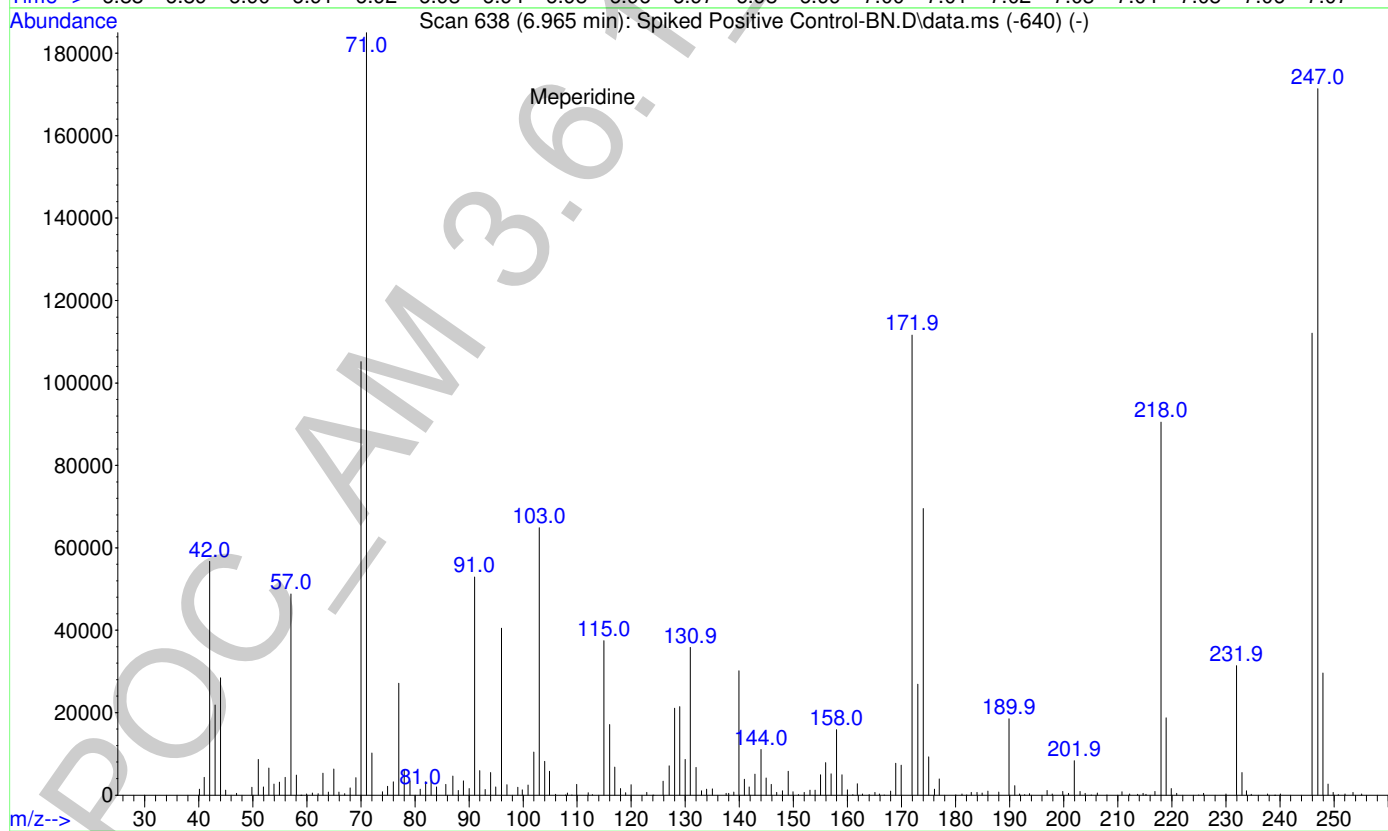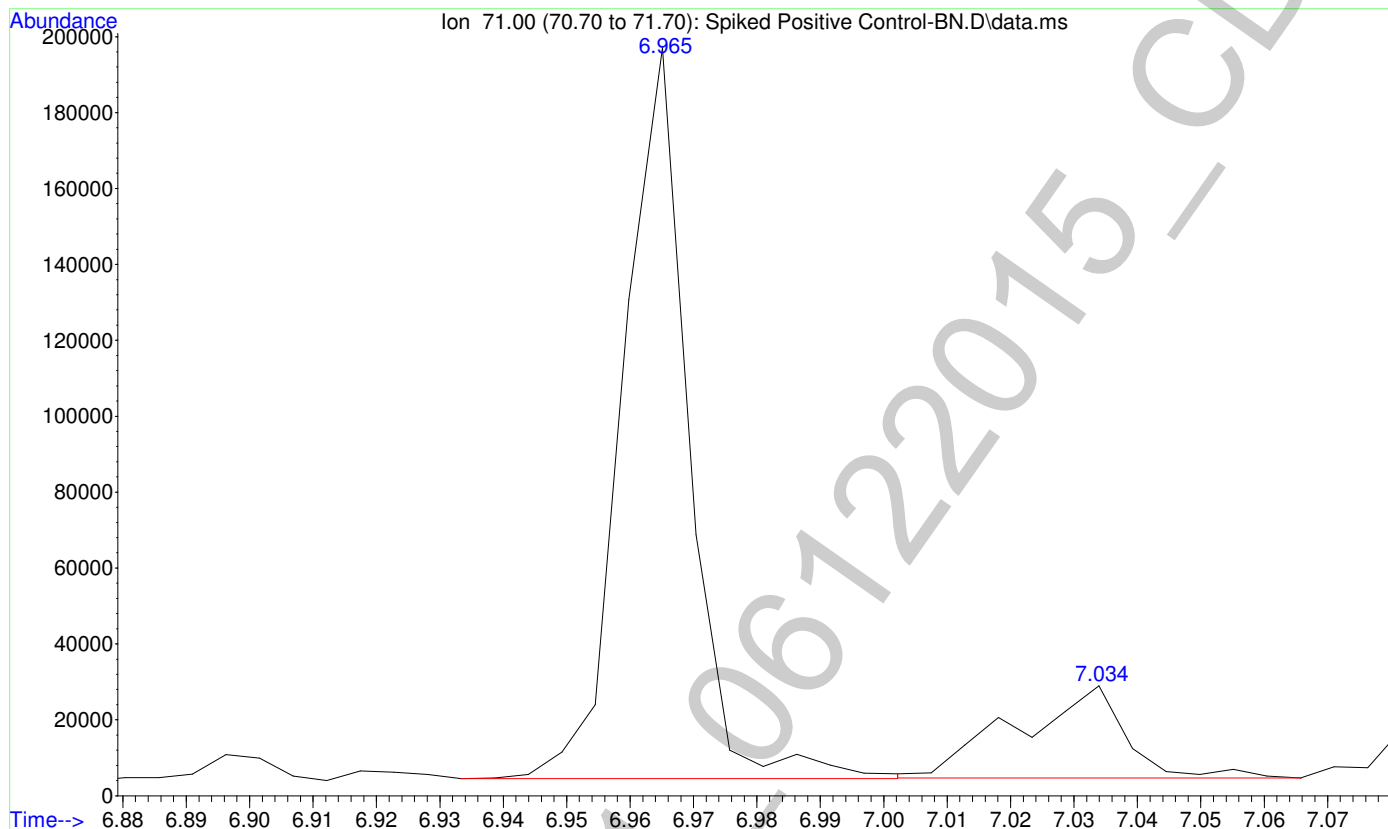



2

File : I:\Celena\061215\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 12 Jun 2015 13:52 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

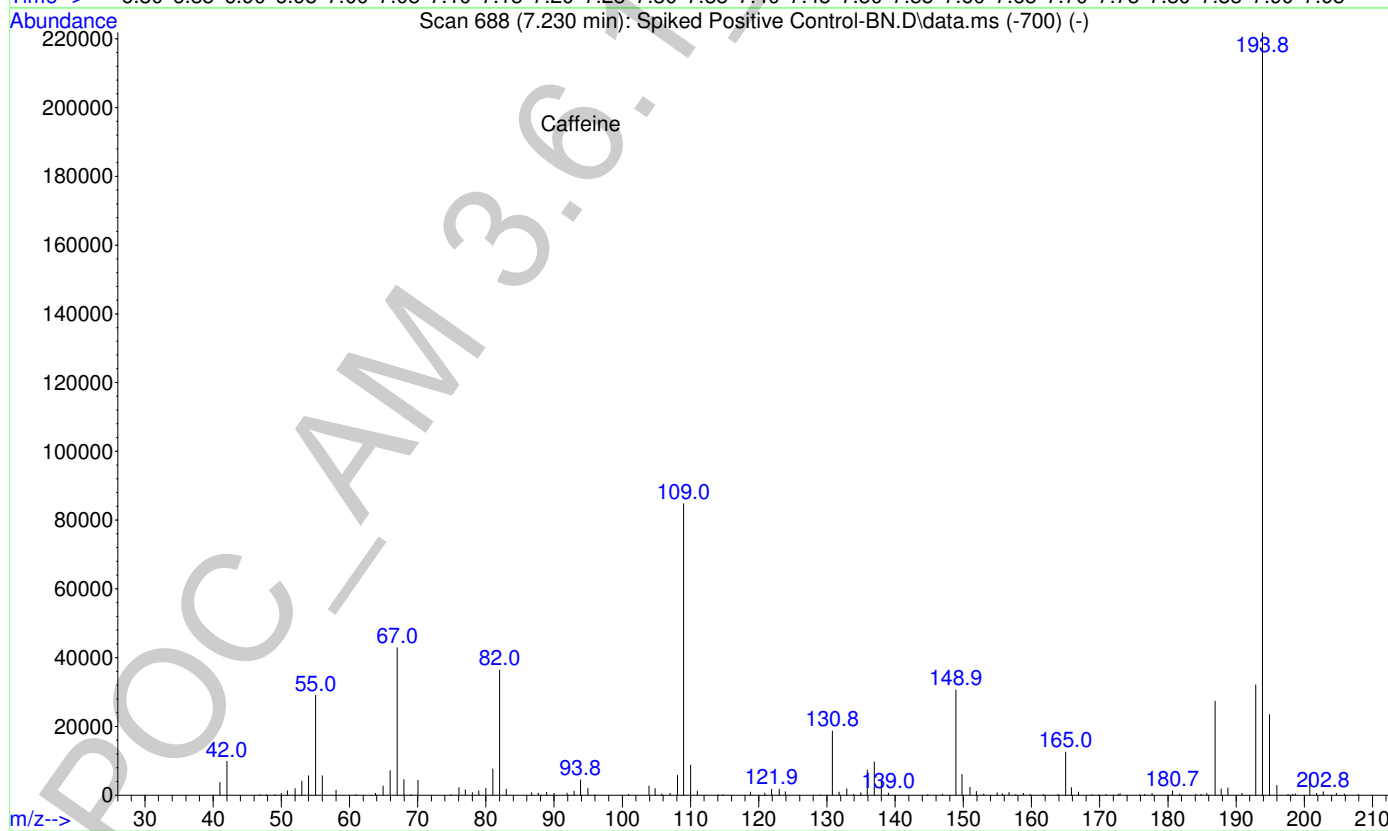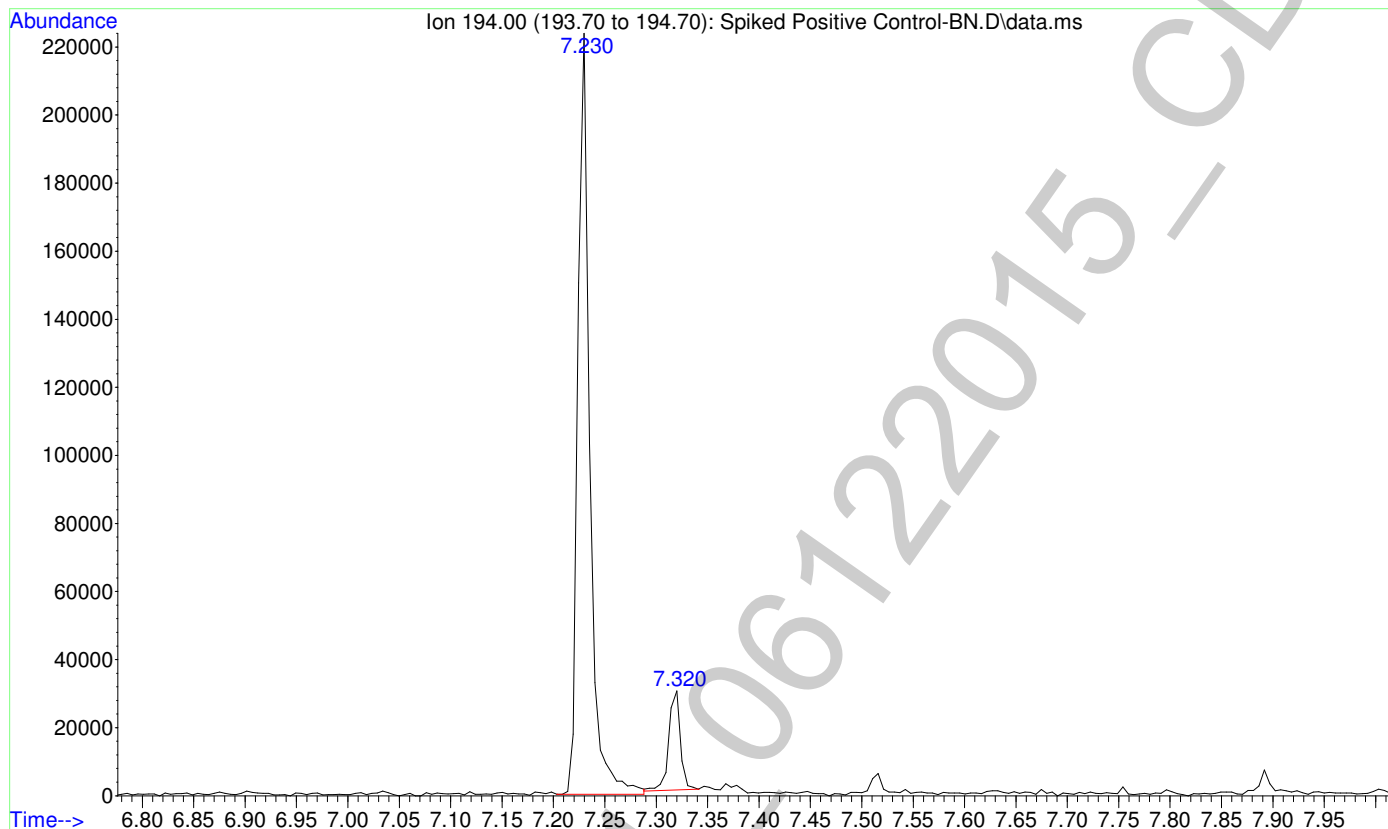



File : I:\Celena\061215\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 12 Jun 2015 13:52 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

2

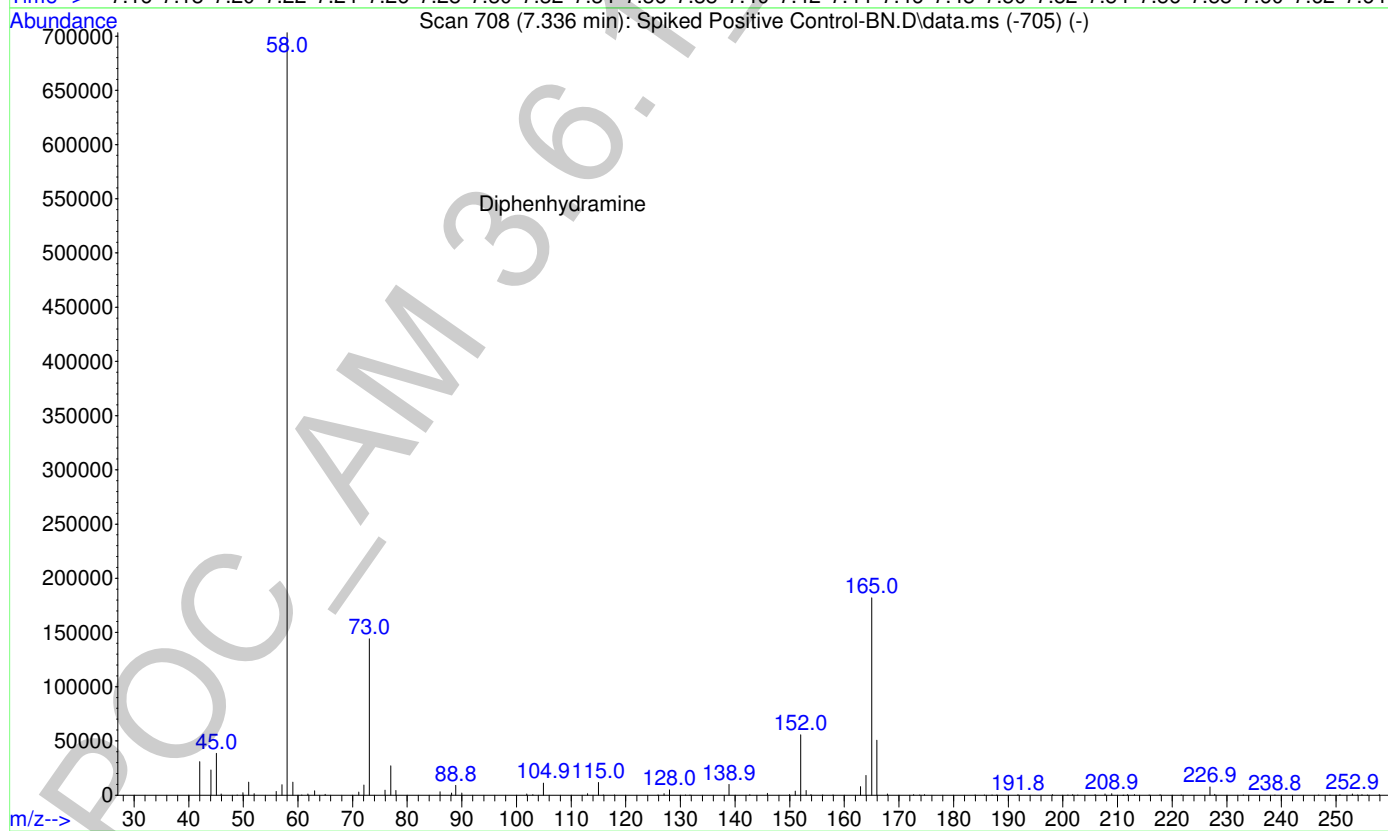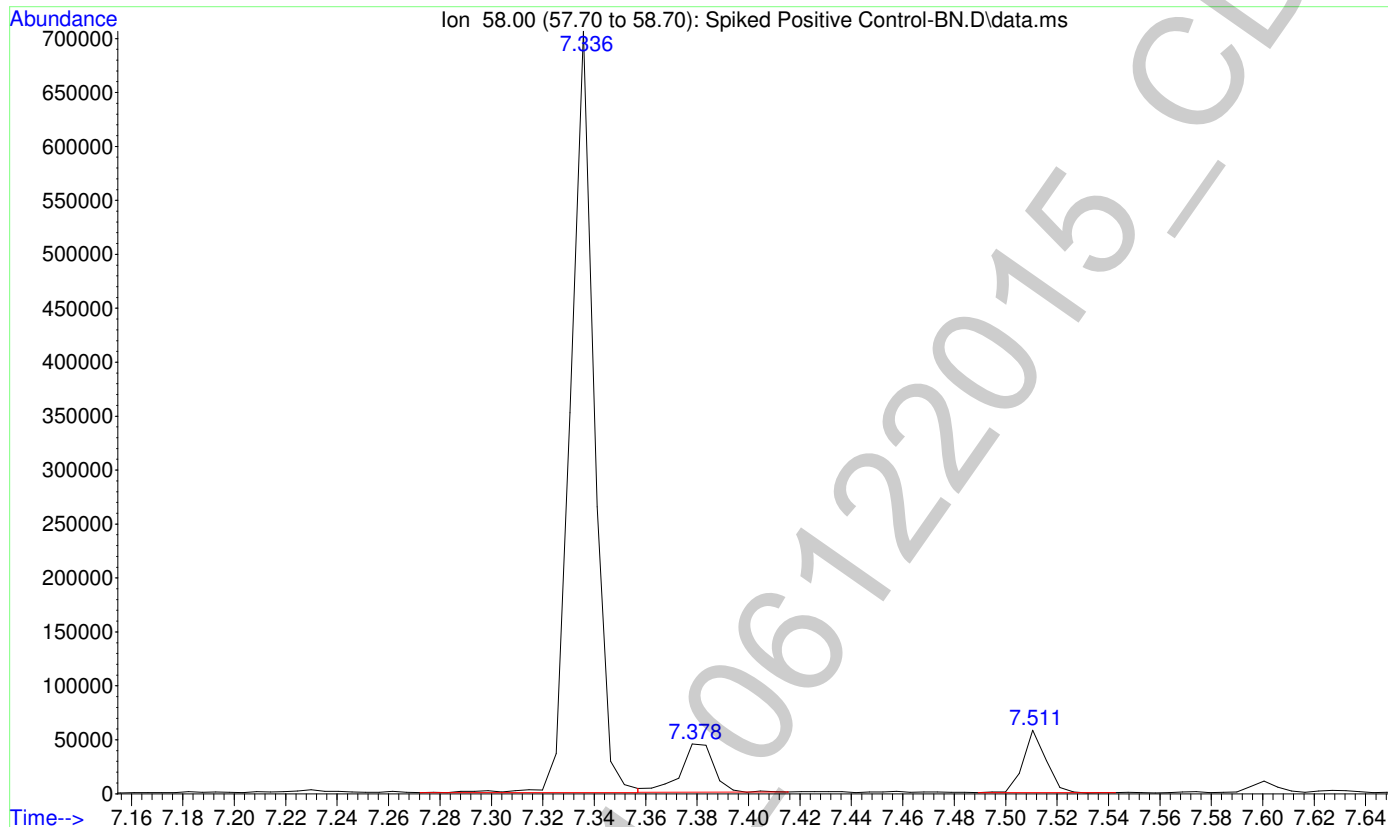



File : I:\Celena\061215\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 12 Jun 2015 13:52 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

g

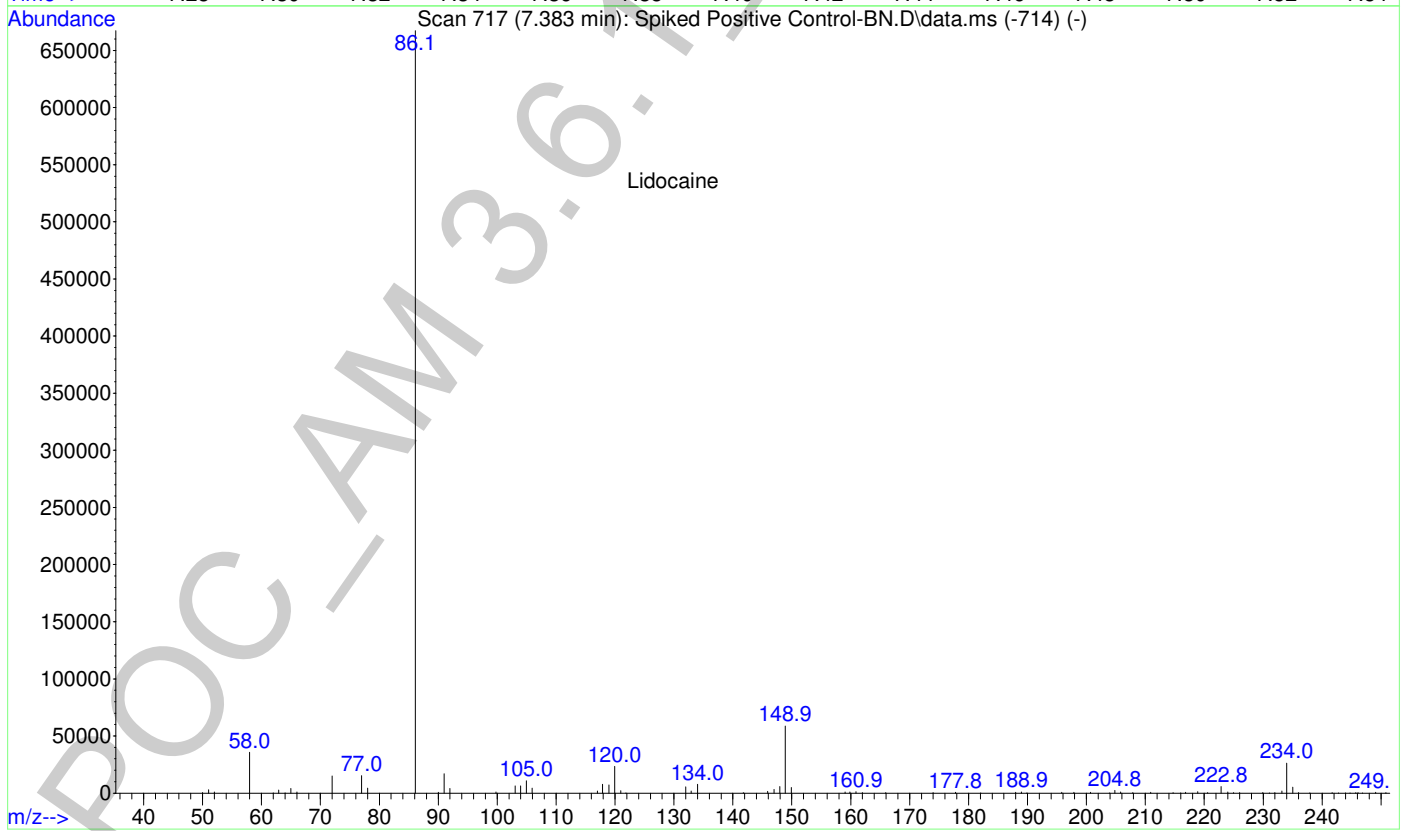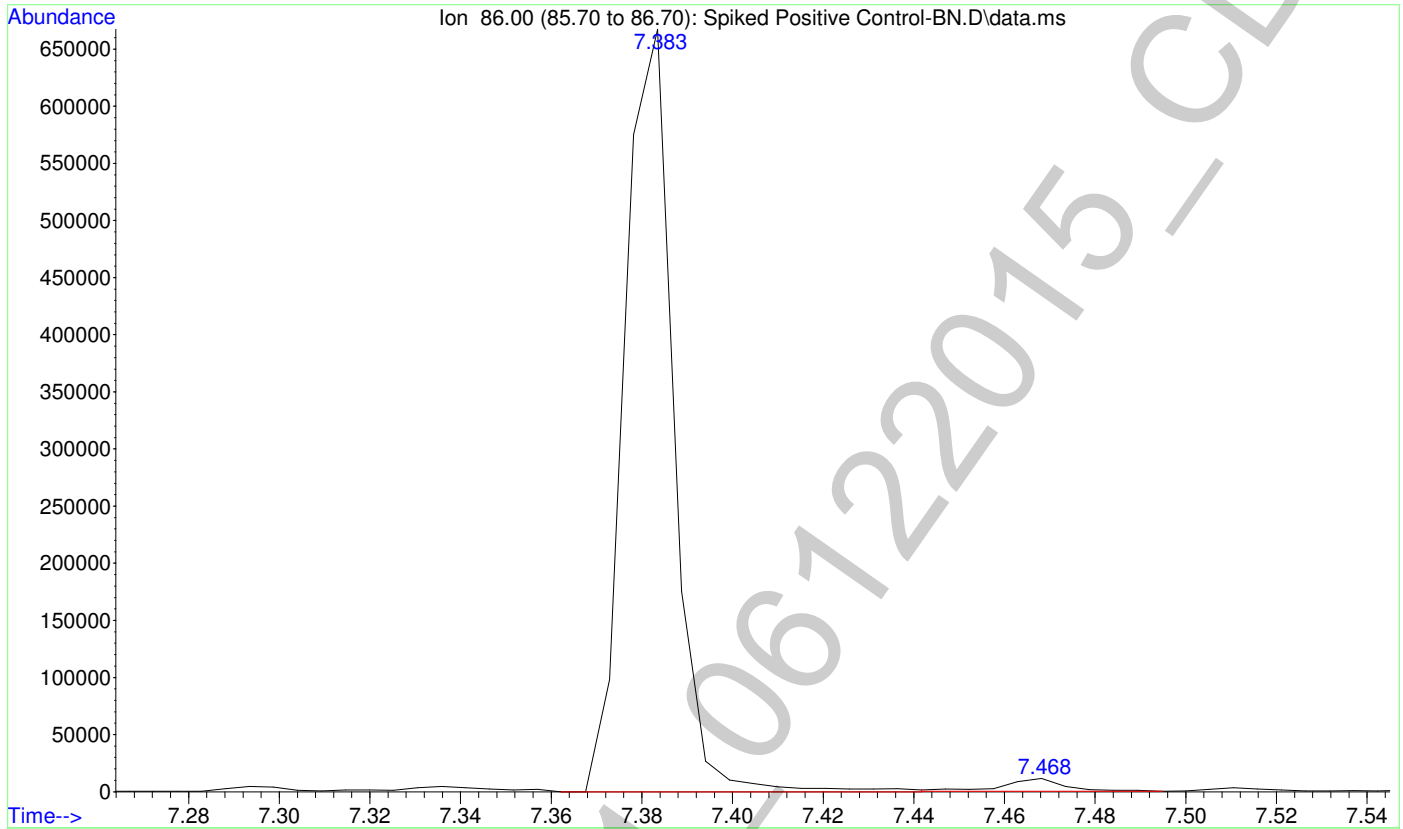



2

File : I:\Celena\061215\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 12 Jun 2015 13:52 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

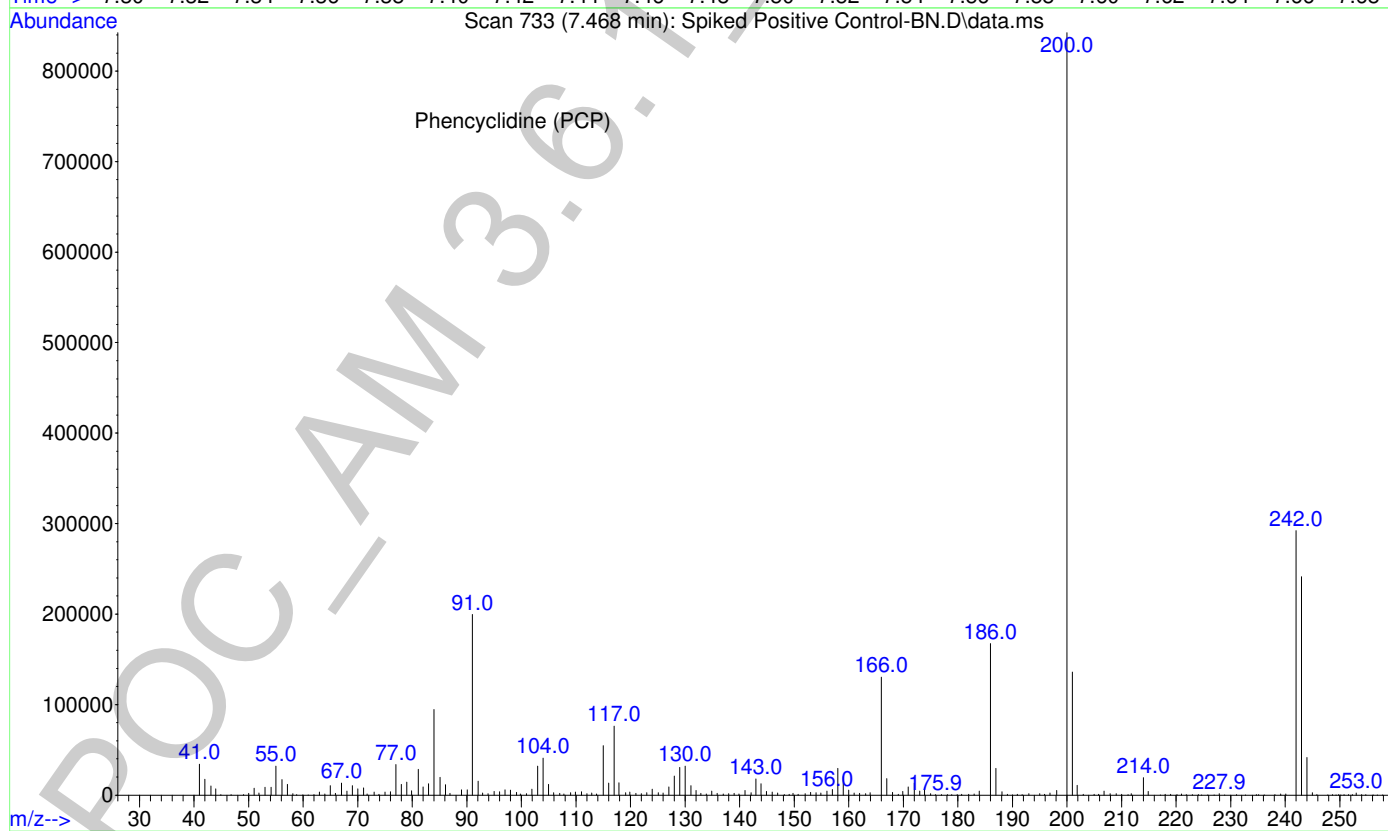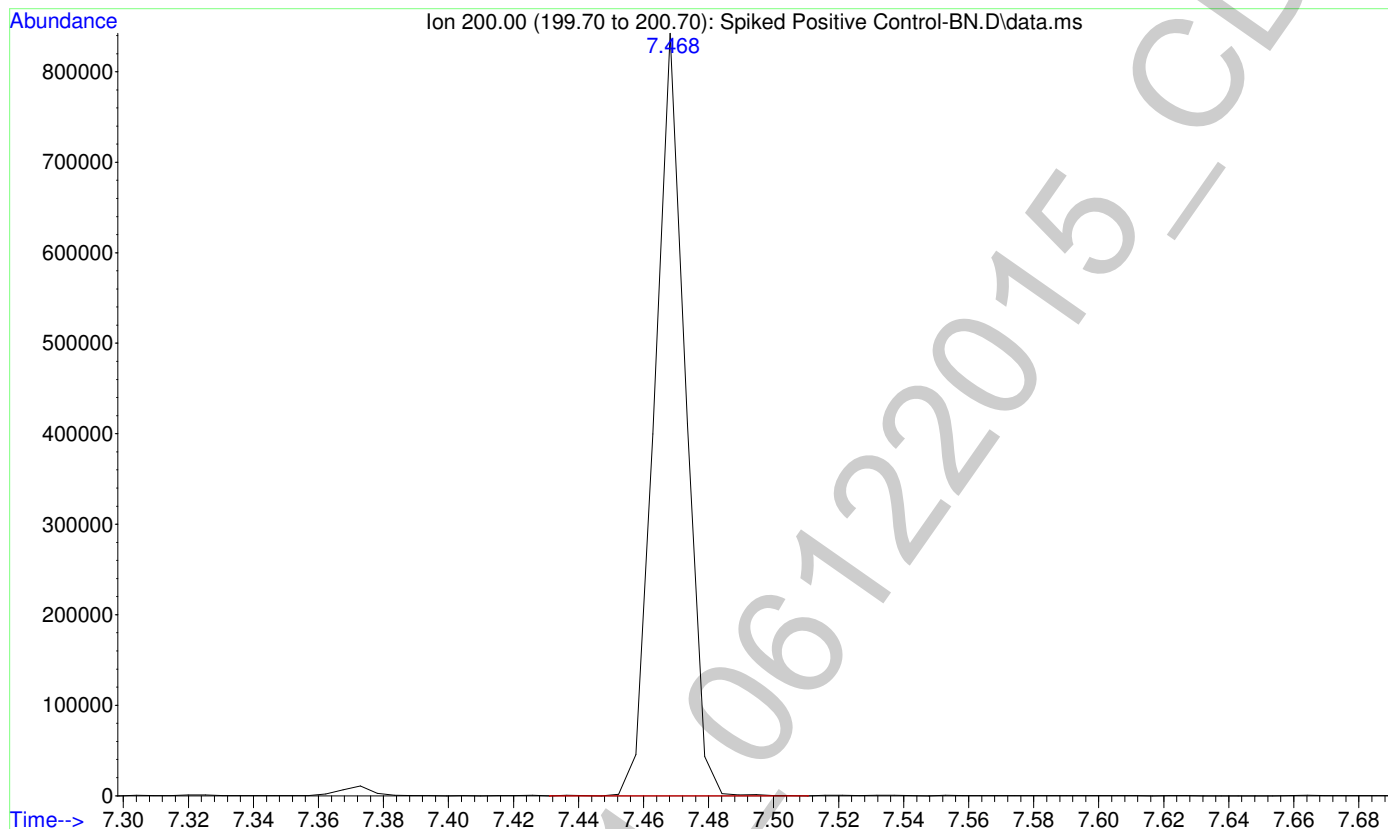



File : I:\Celena\061215\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 12 Jun 2015 13:52 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

6

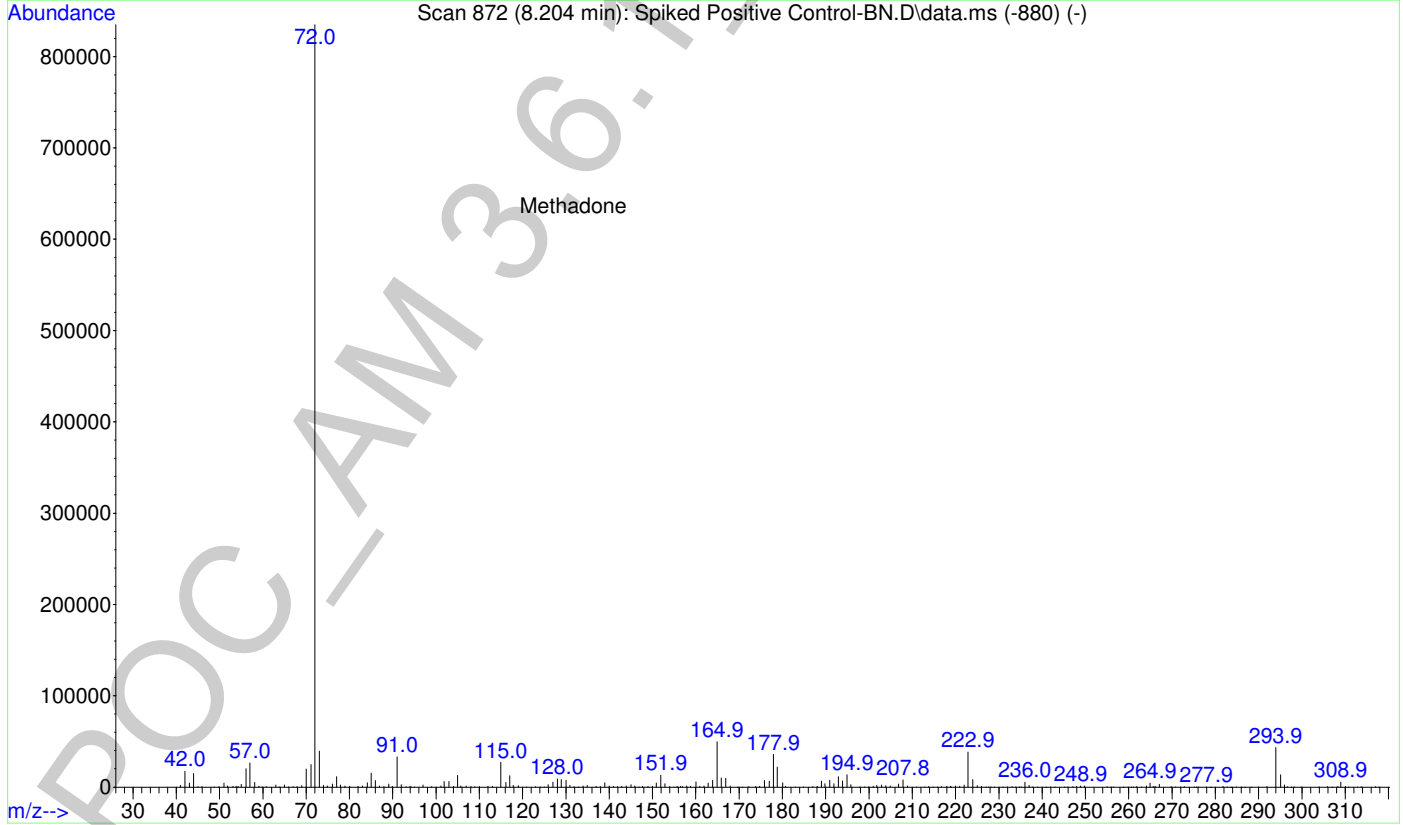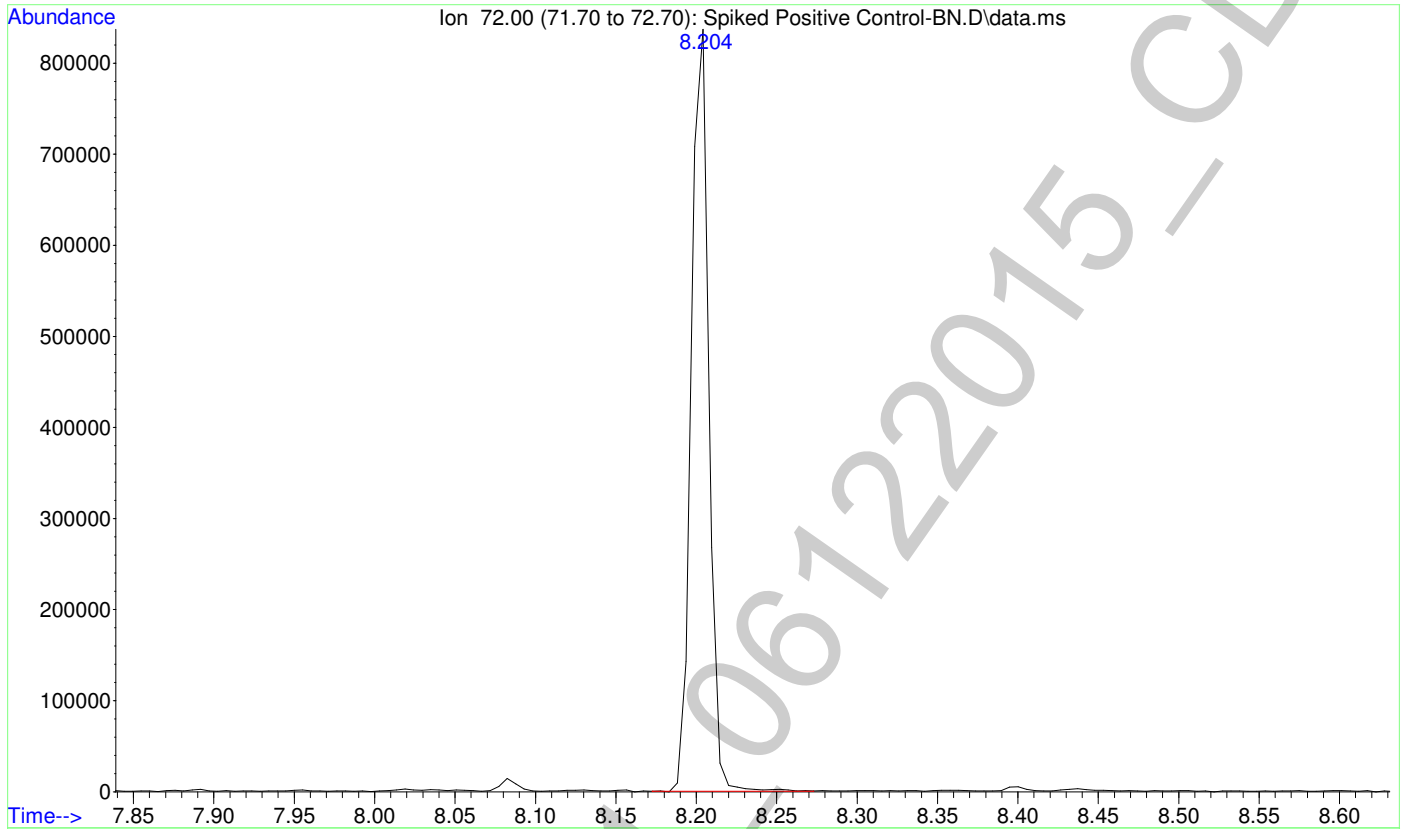



2

File : I:\Celena\061215\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 12 Jun 2015 13:52 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

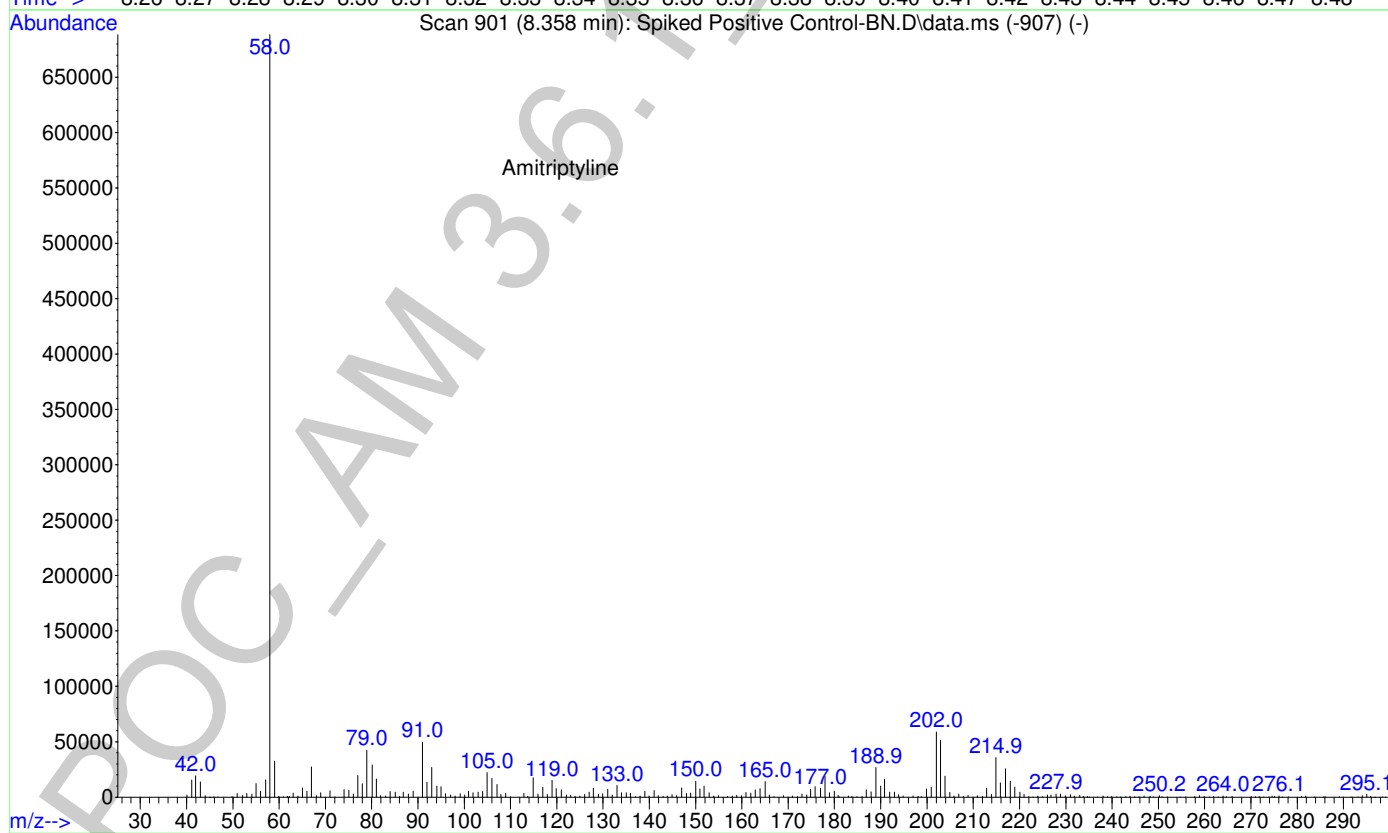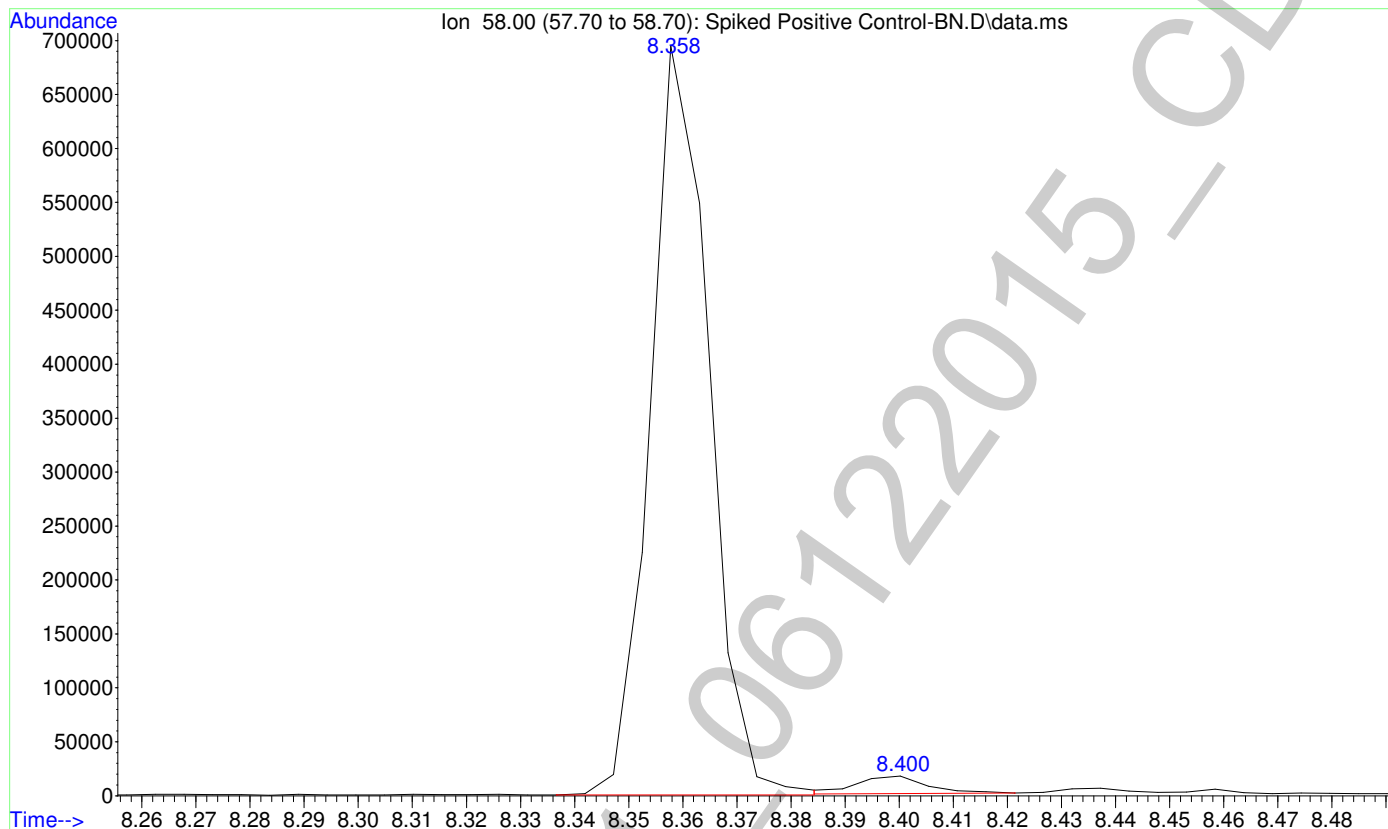



File : I:\Celena\061215\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 12 Jun 2015 13:52 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

6

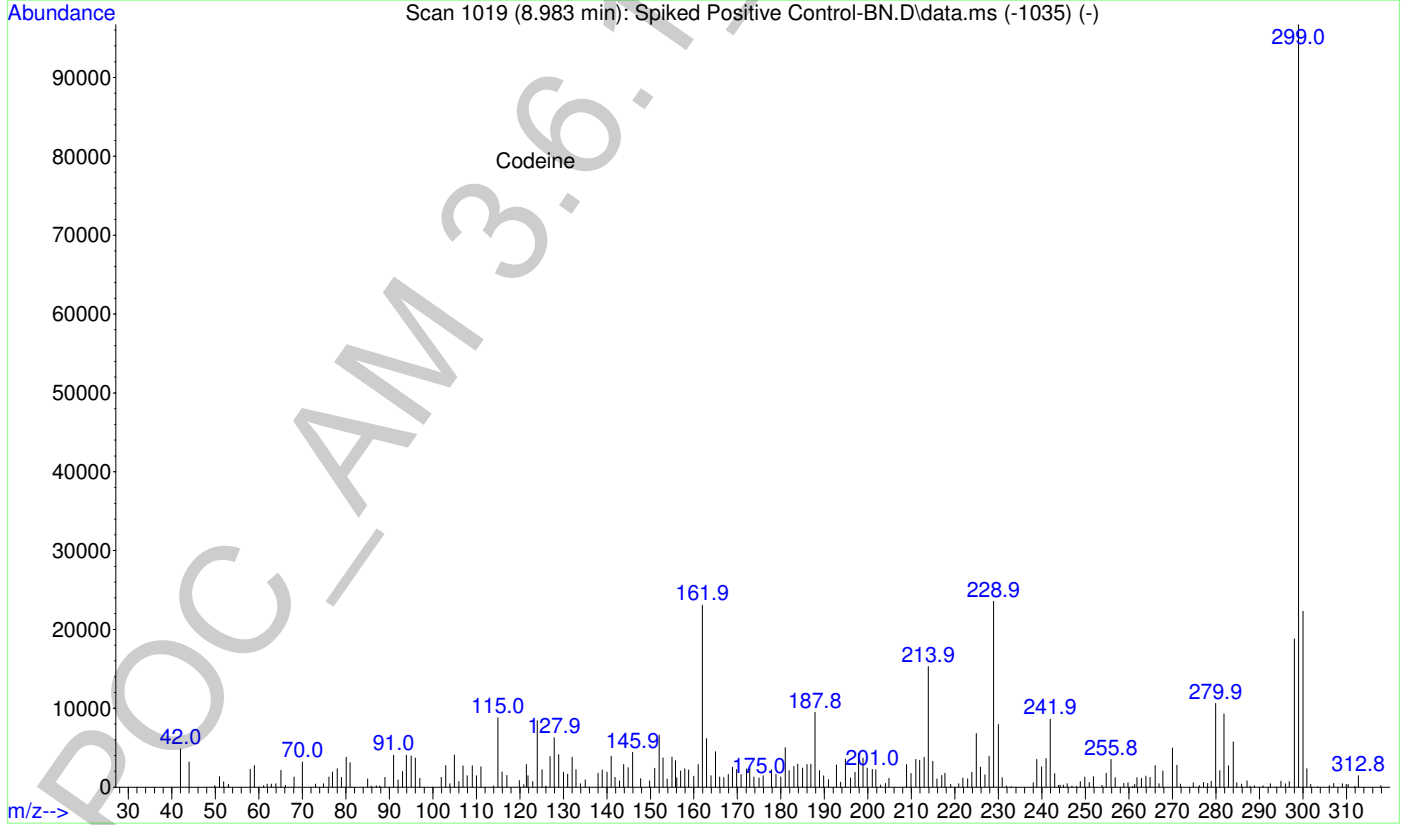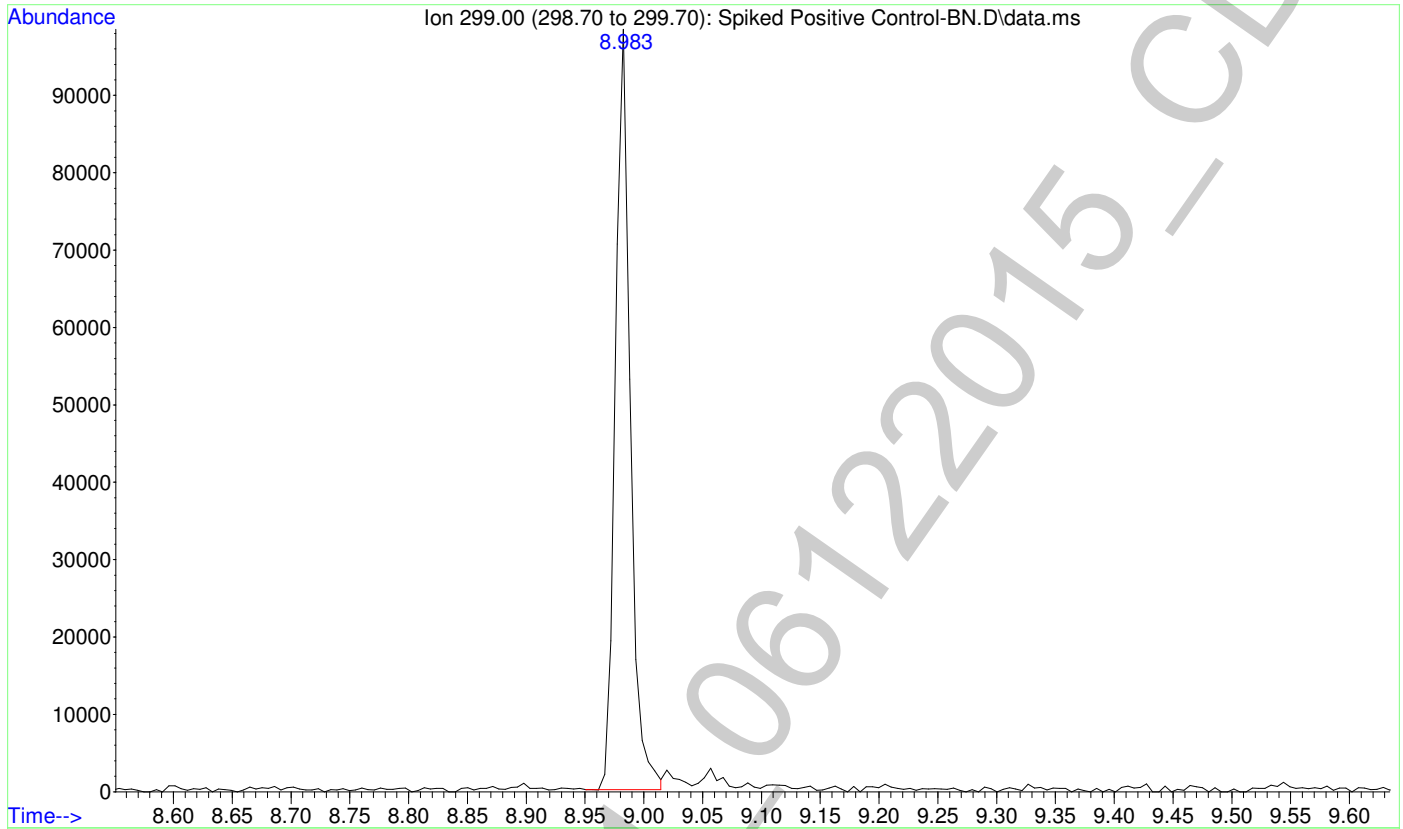

2

File : I:\Celena\061215\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 12 Jun 2015 13:52 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name : Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number : 2

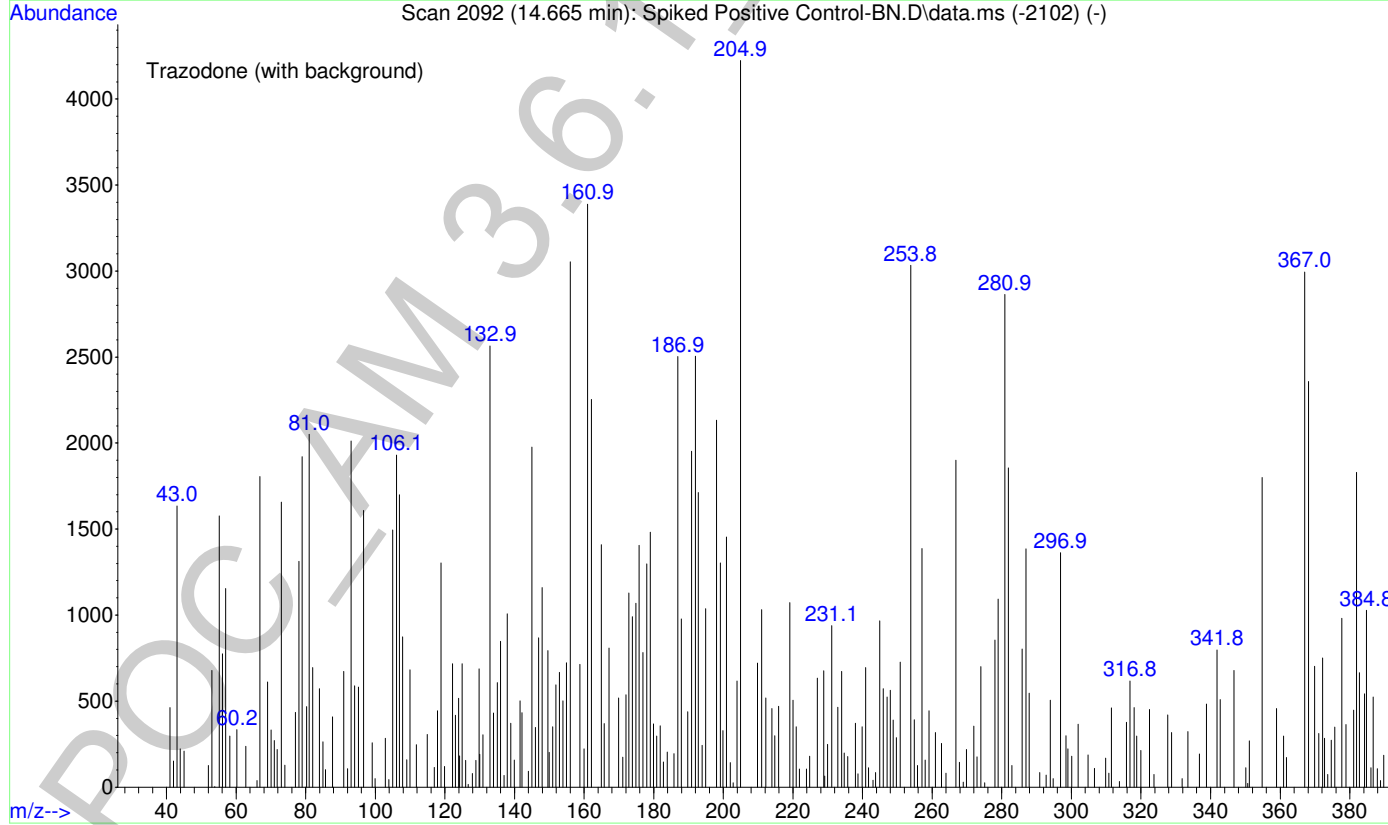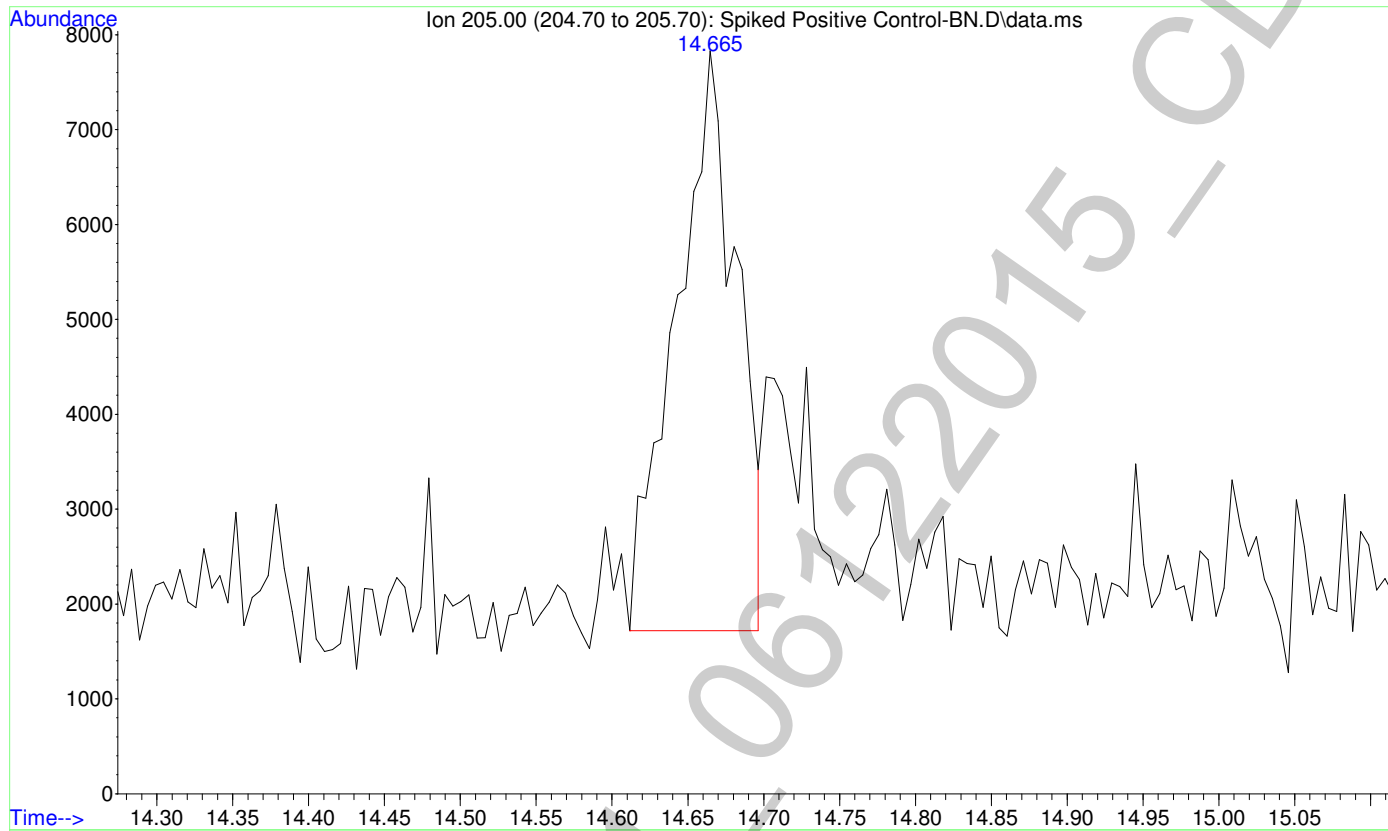

2

Analytical Method 3.6.1 & 3.6.7 QA Check List

Run Start Date: 06/12/15

Analyst: CS

(Long GC/MS temperature program)

Positive Control Compound List

- Methamphetamine
- Nicotine
- Meperidine
- Caffeine
- Diphenhydramine
- Lidocaine
- PCP
- Methadone
- Amitriptyline
- Codeine
- Trazodone

Internal Standards


- Benzphetamine
- Papaverine

Optional back extraction **not** performed.
Reconstituted in MeOH.

POC_AM 3.6.1_06122015_CDS



6

File :I:\Celena\061215\Negative Control-BNr.D
Operator : ISP\datastor
Acquired : 12 Jun 2015 15:11 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1
Vial Number: 1

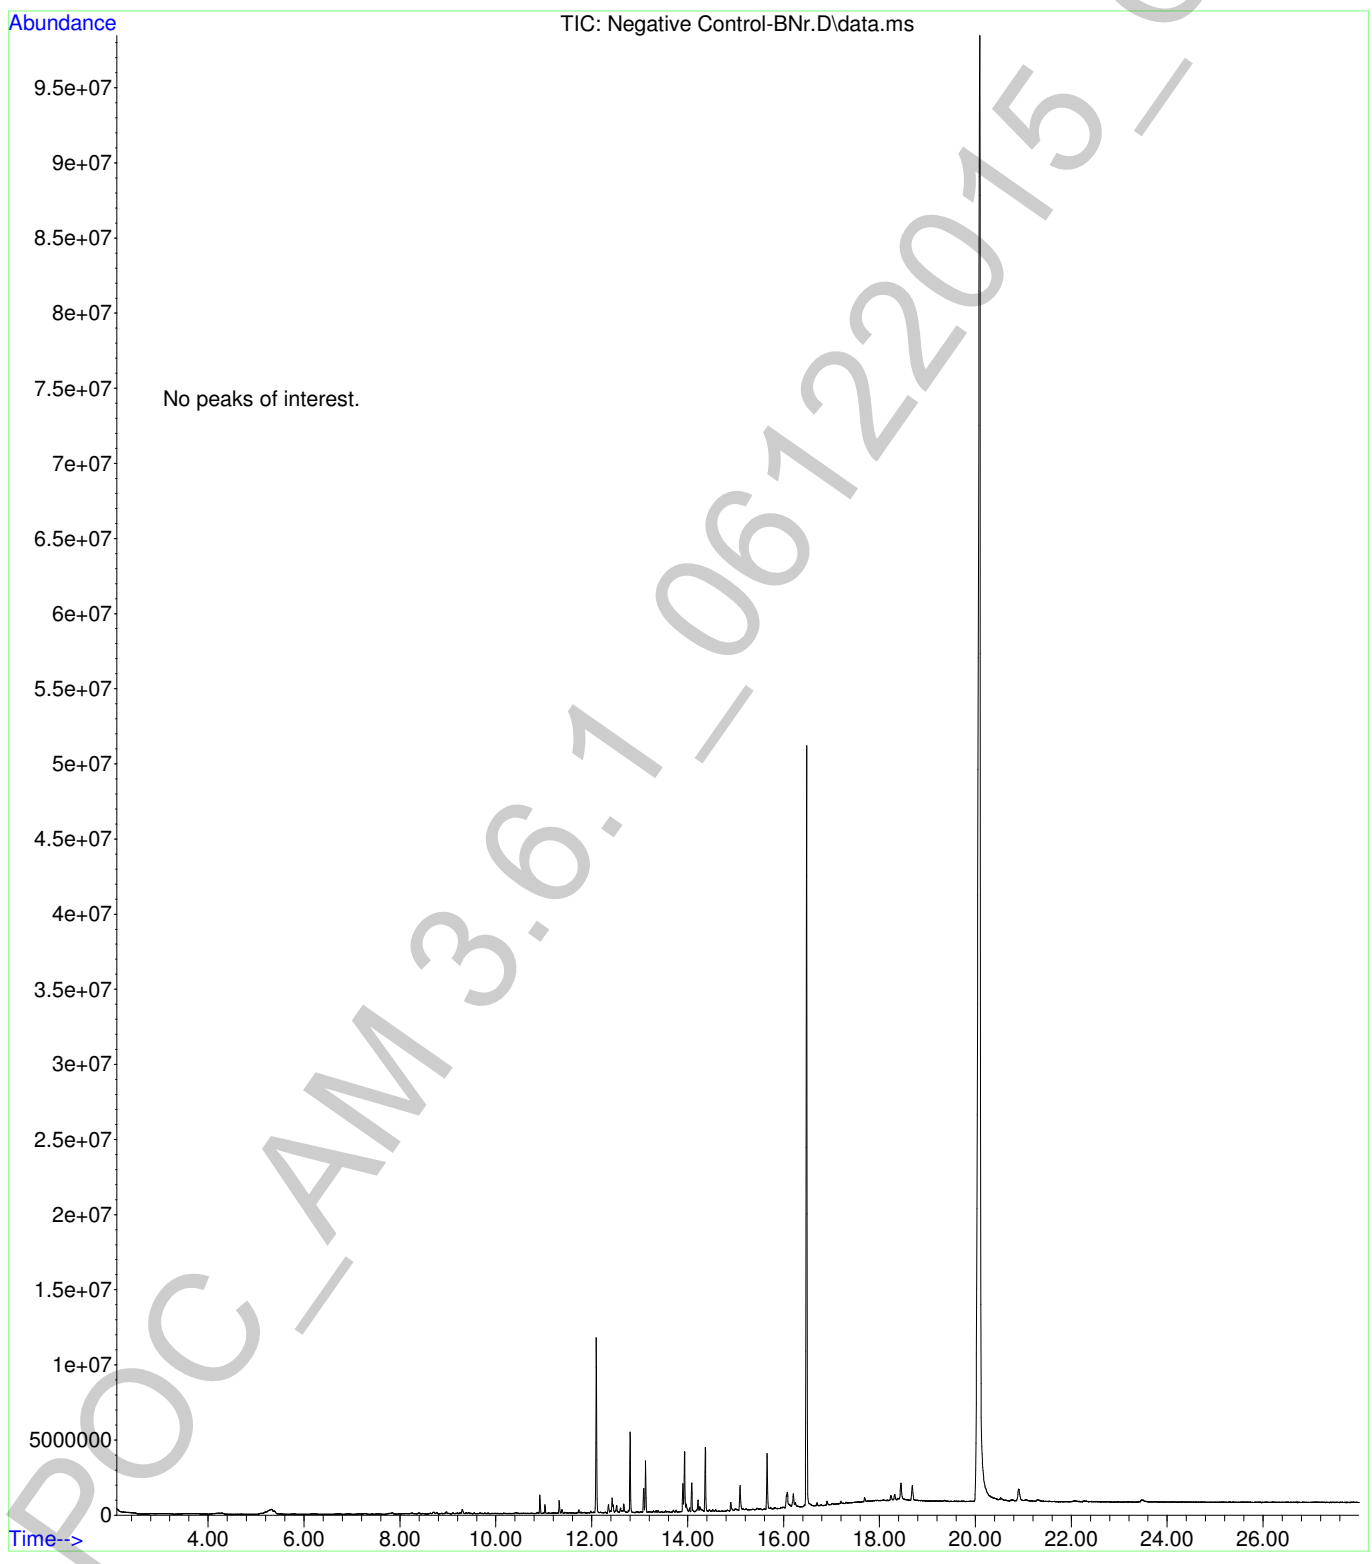



2

File : I:\Celena\061215\Negative Control-BN.D
Operator : ISP\datastor
Acquired : 12 Jun 2015 13:29 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1
Vial Number: 1

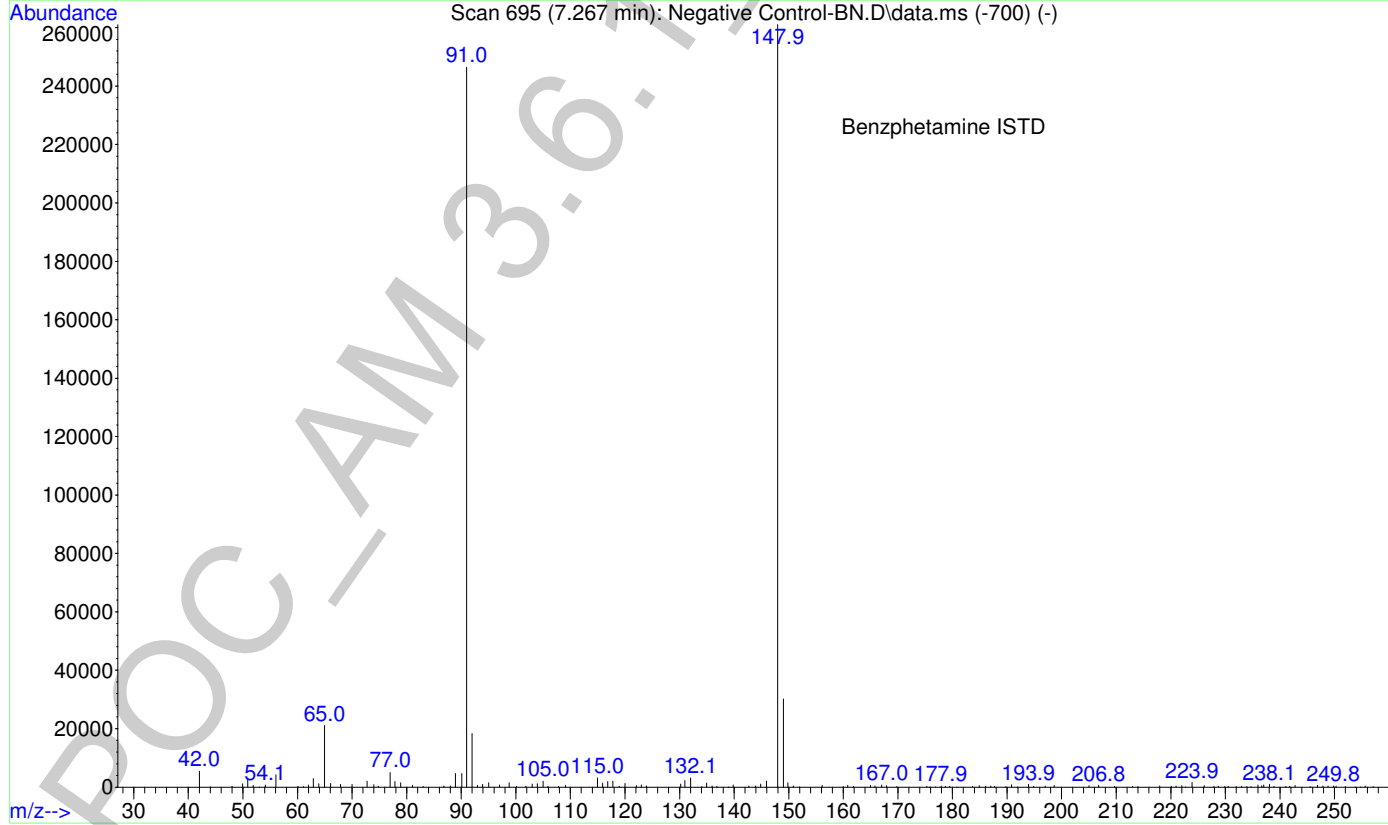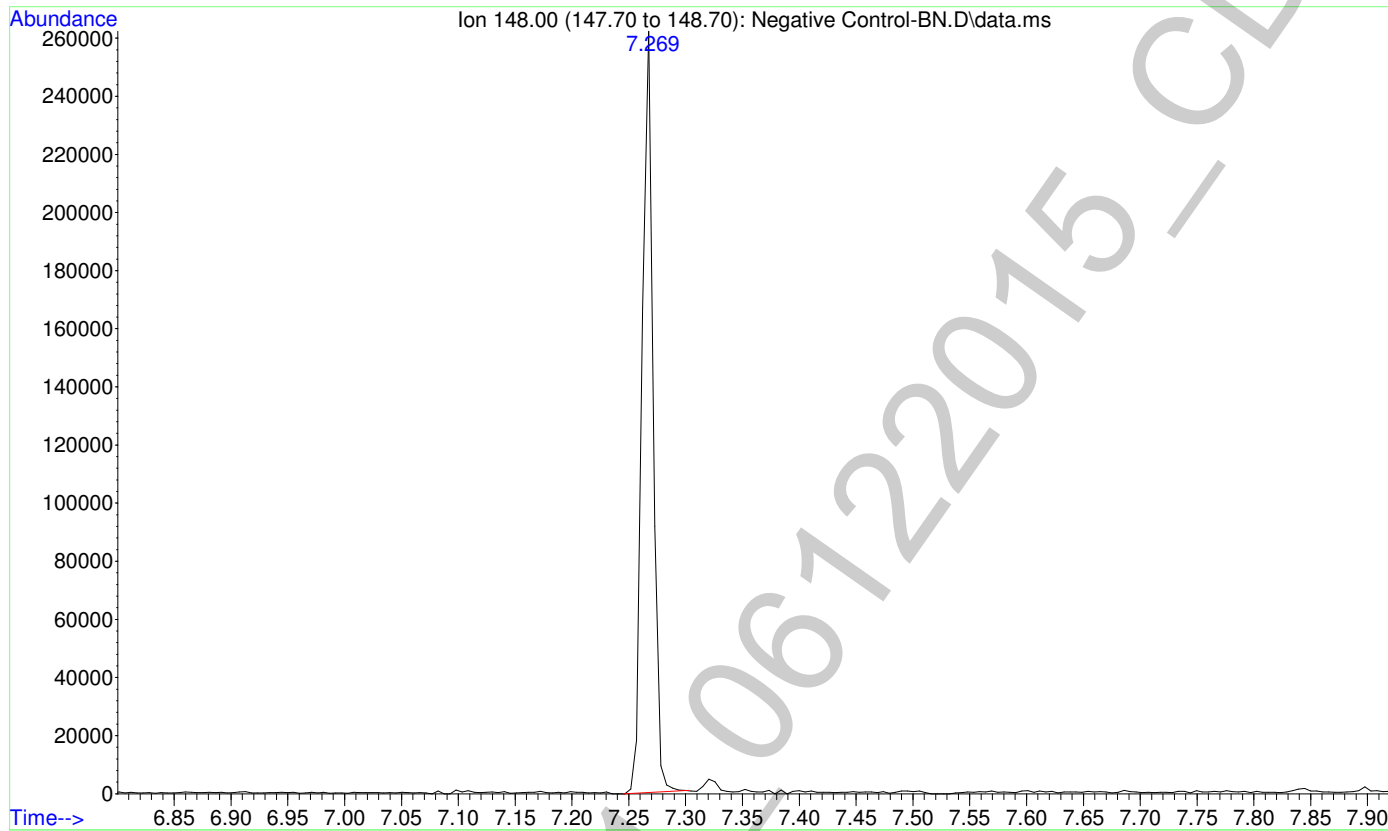


2

File : I:\Celena\061215\Negative Control-BNr.D
Operator : ISP\datastor
Acquired : 12 Jun 2015 15:11 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1
Vial Number: 1

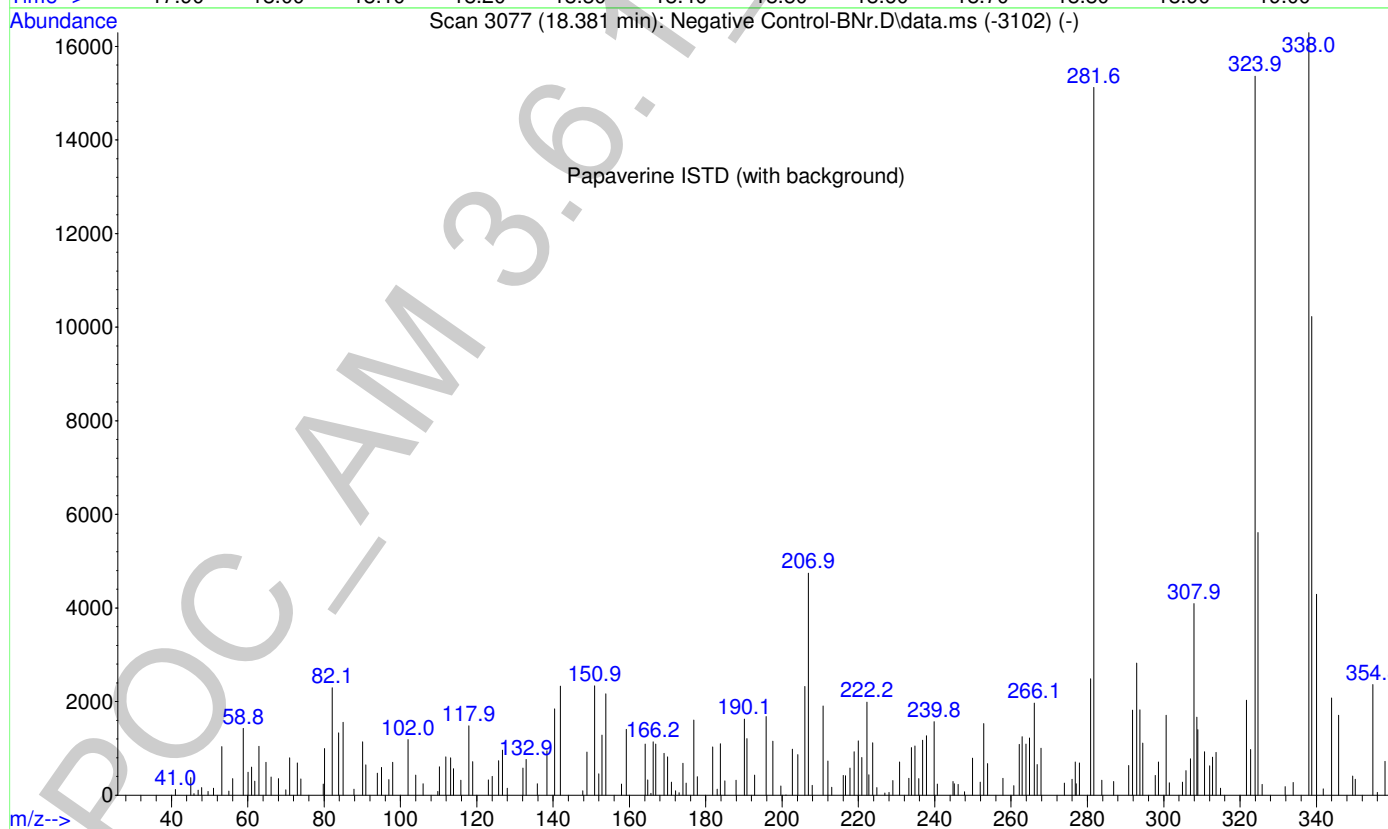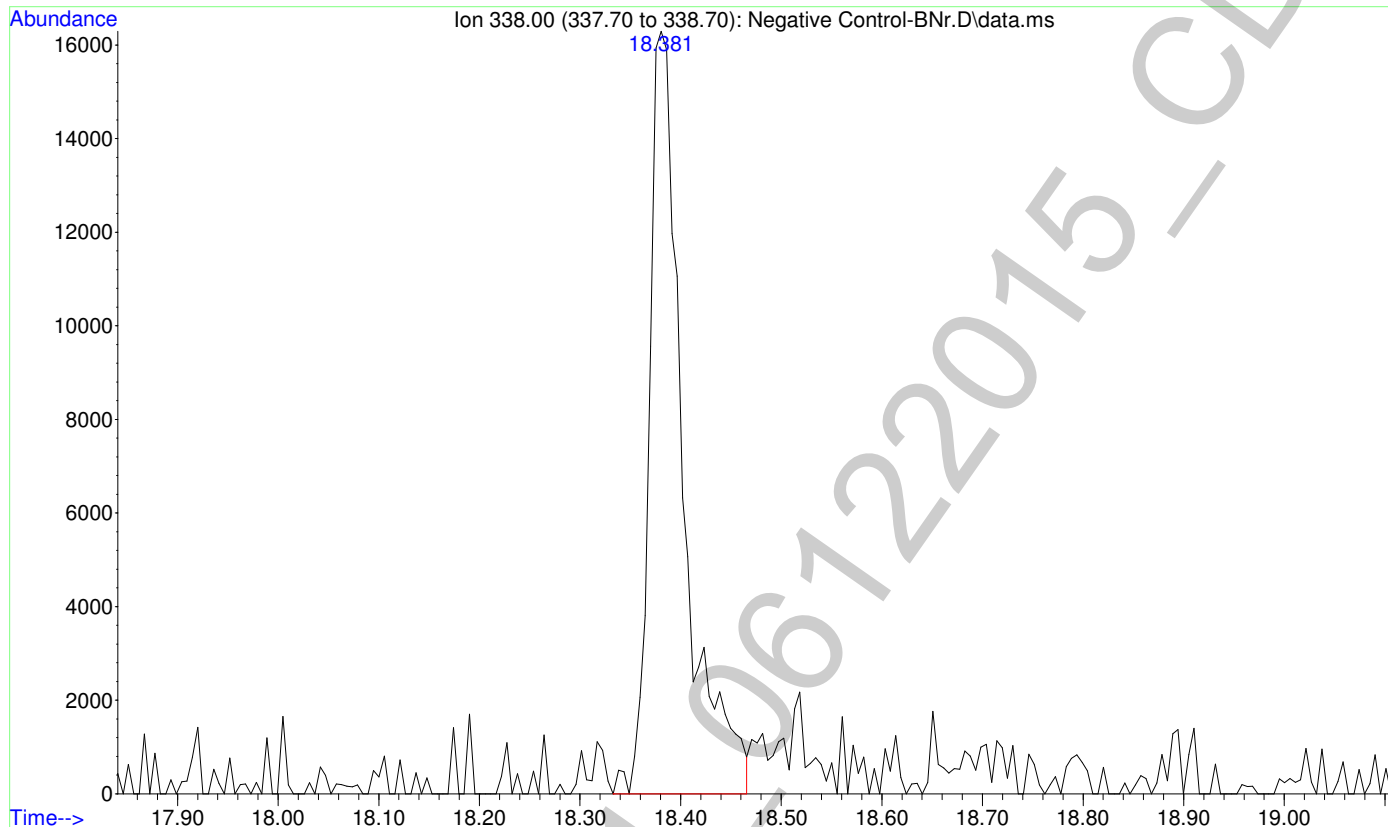



6

File :C:\MyFiles\cshrum\Desktop\Data\061215\Spiked Positive Contro
... 1-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 12 Jun 2015 15:45 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

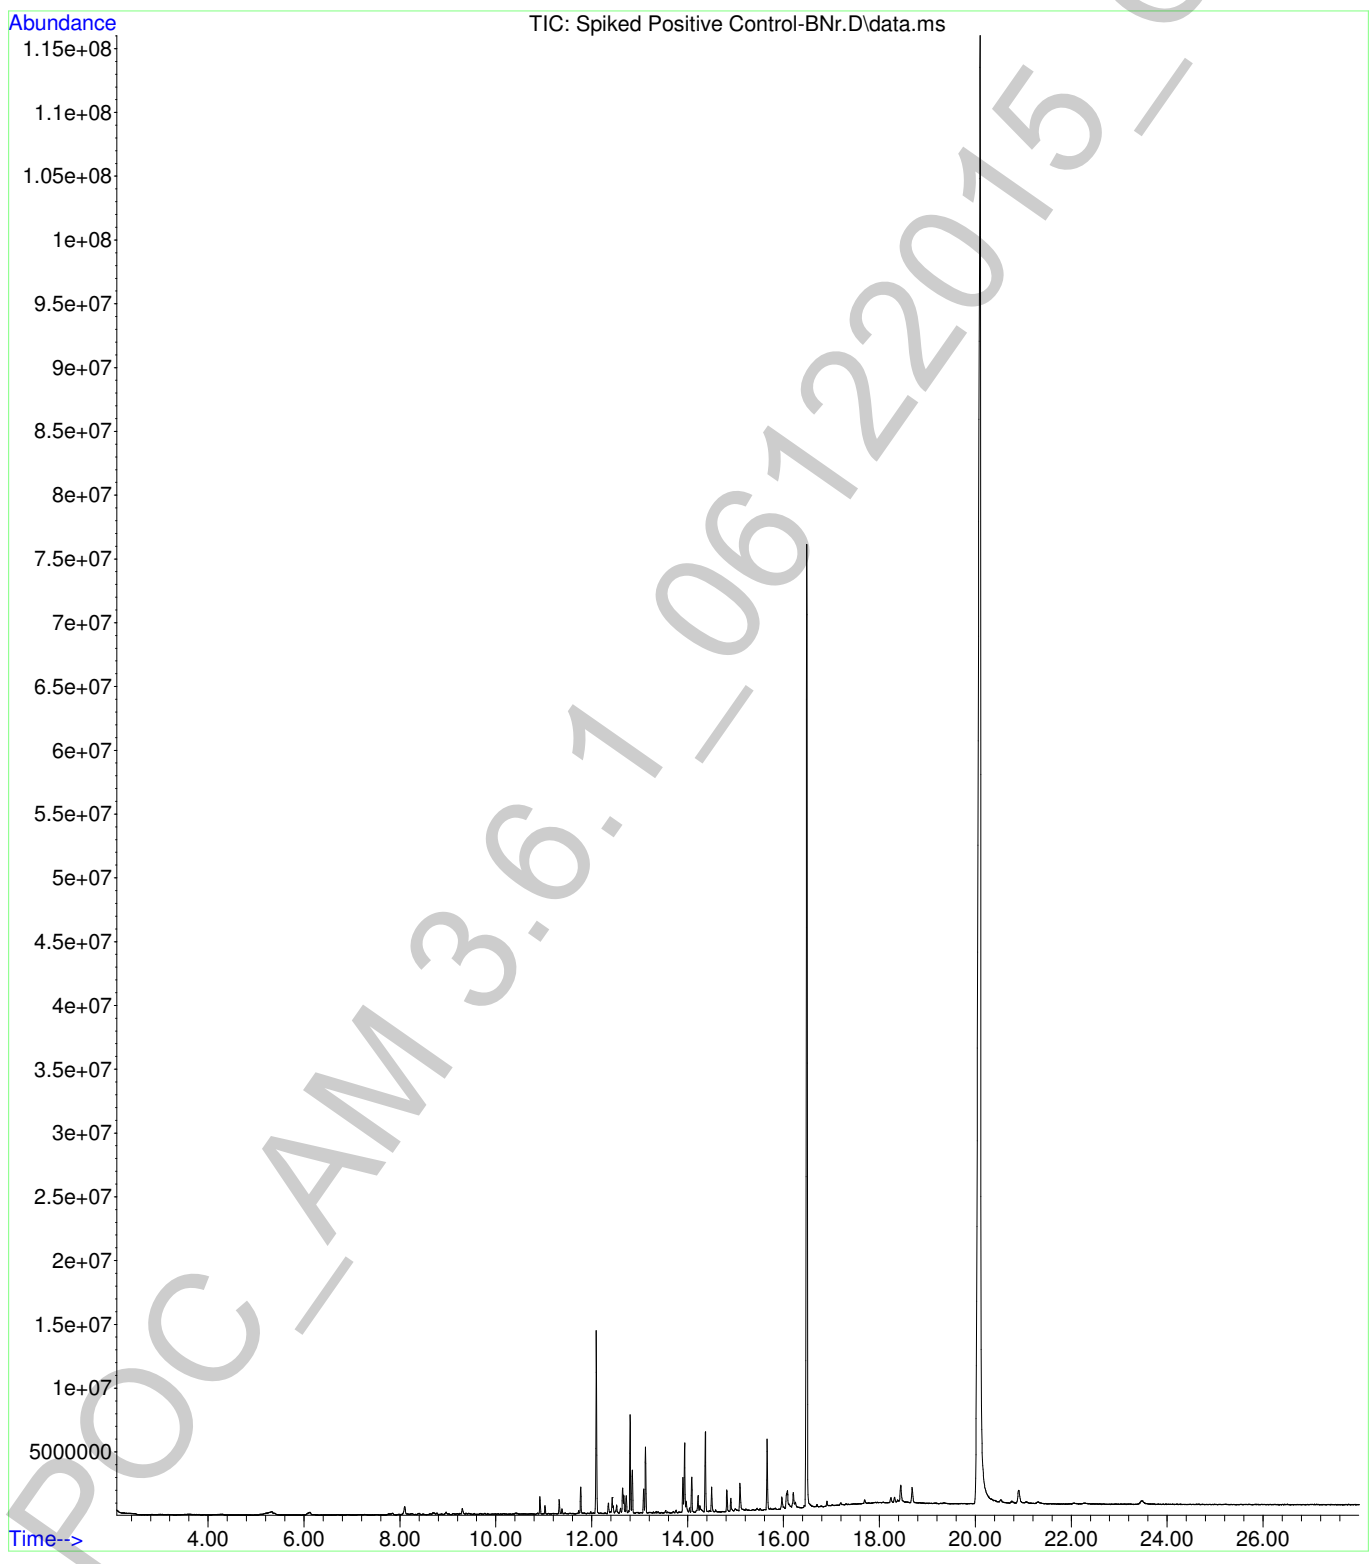



2

File : I:\Celena\061215\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 12 Jun 2015 15:45 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

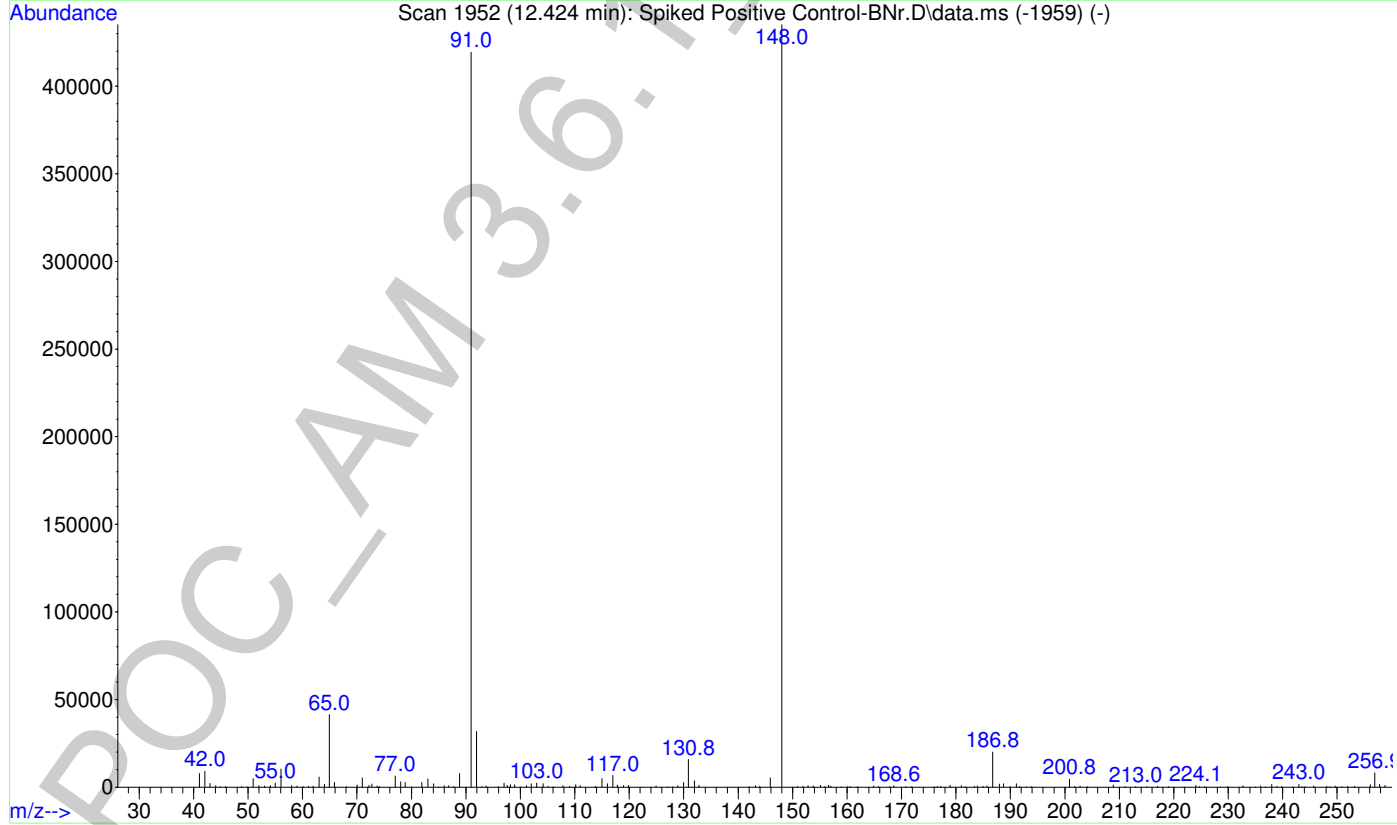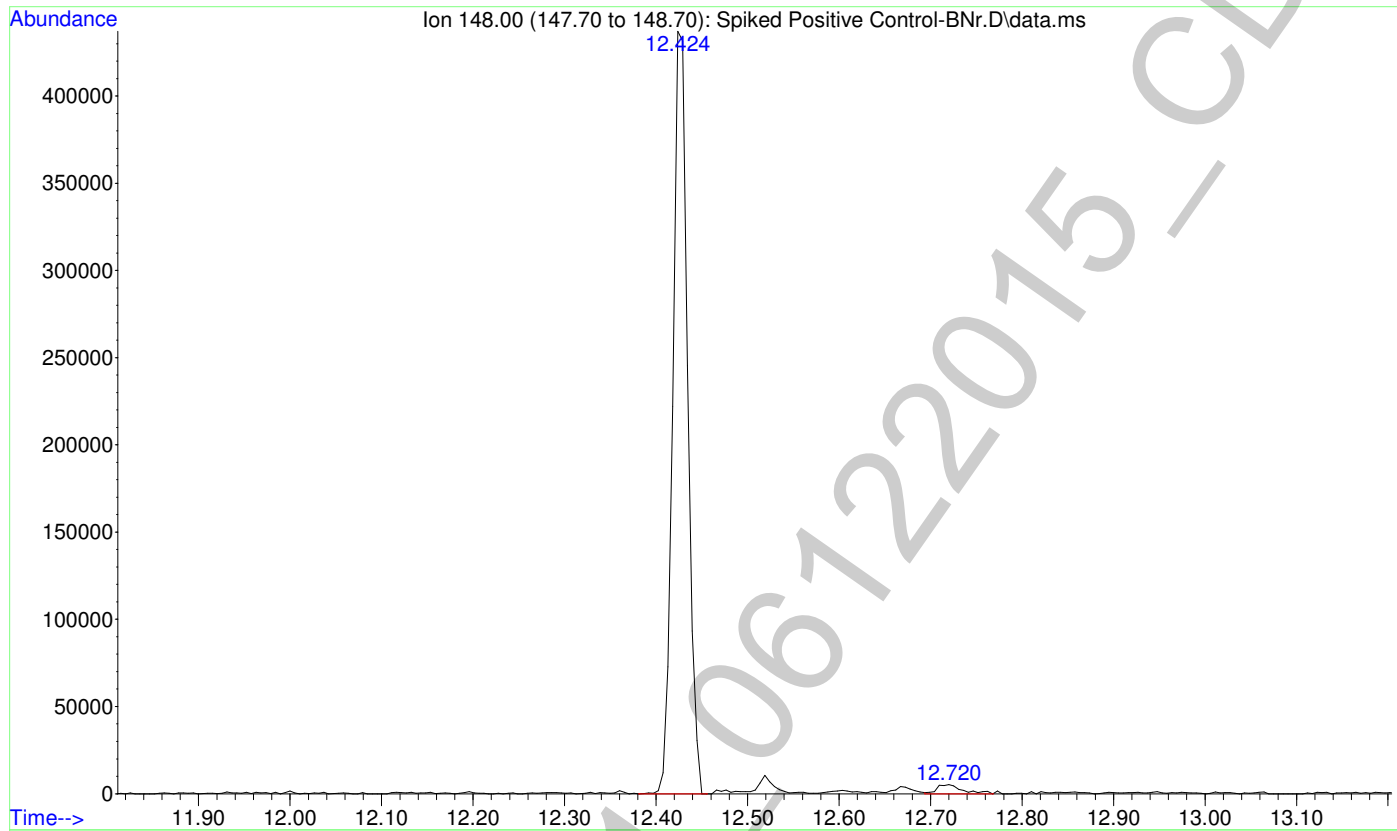



2

File : I:\Celena\061215\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 12 Jun 2015 15:45 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

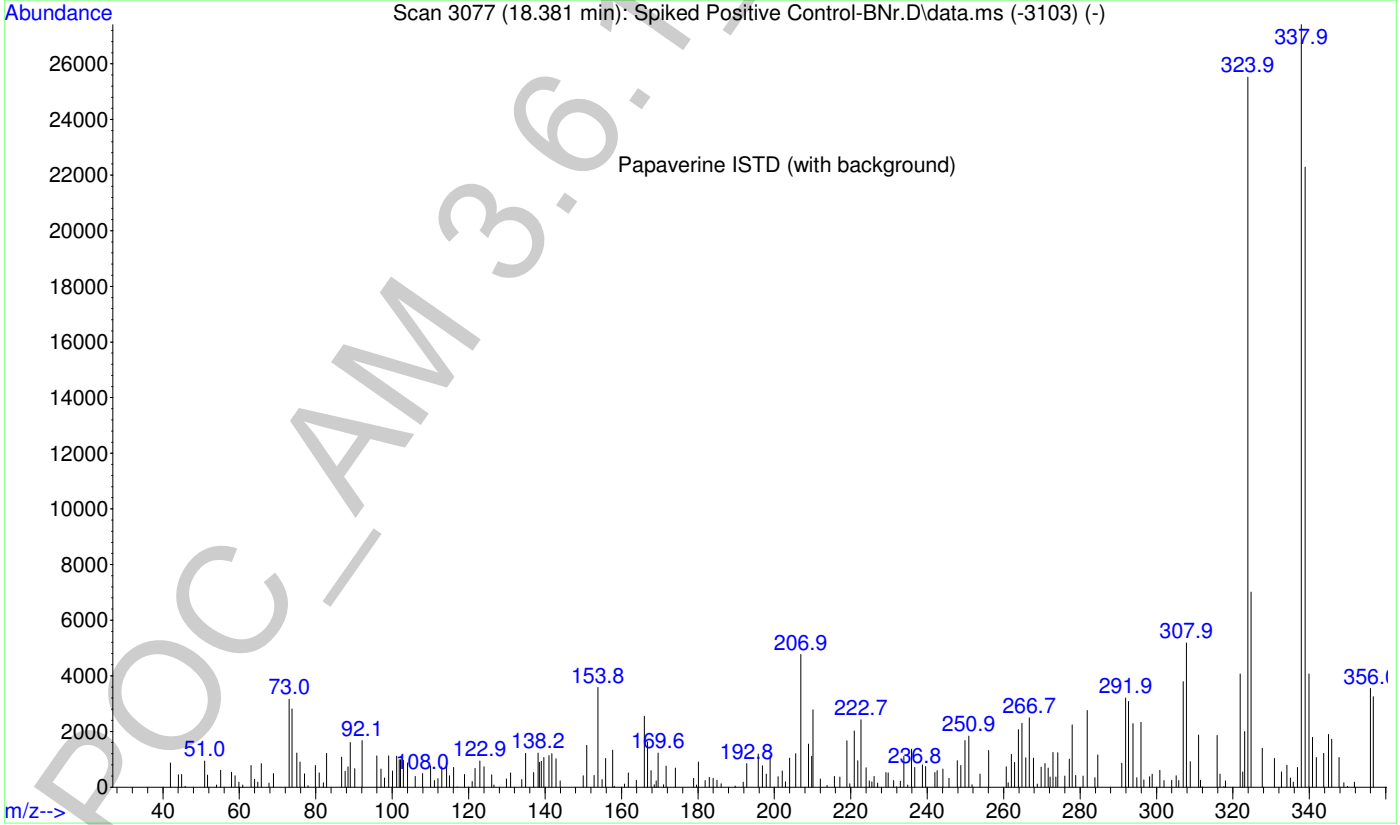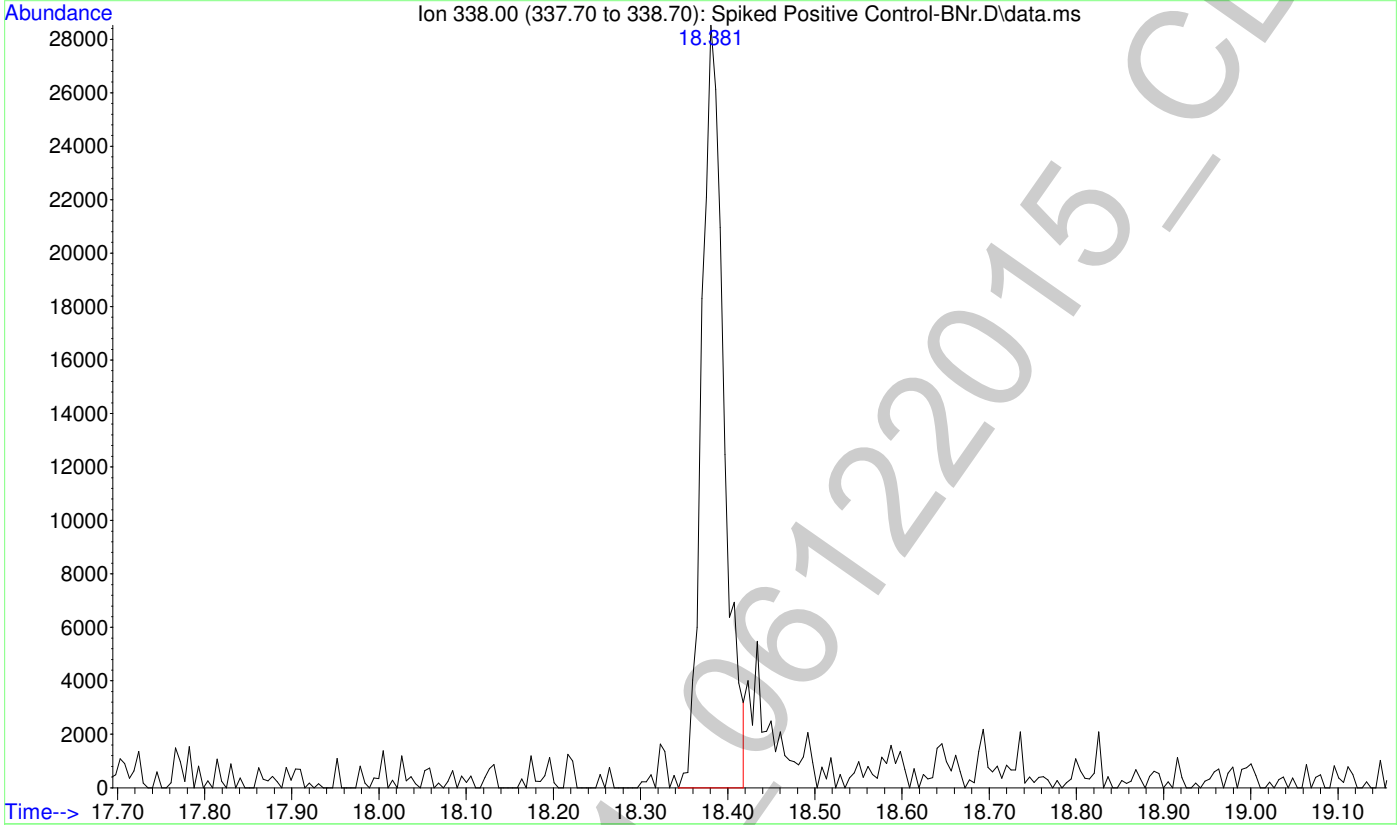



2

File : I:\Celena\061215\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 12 Jun 2015 15:45 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

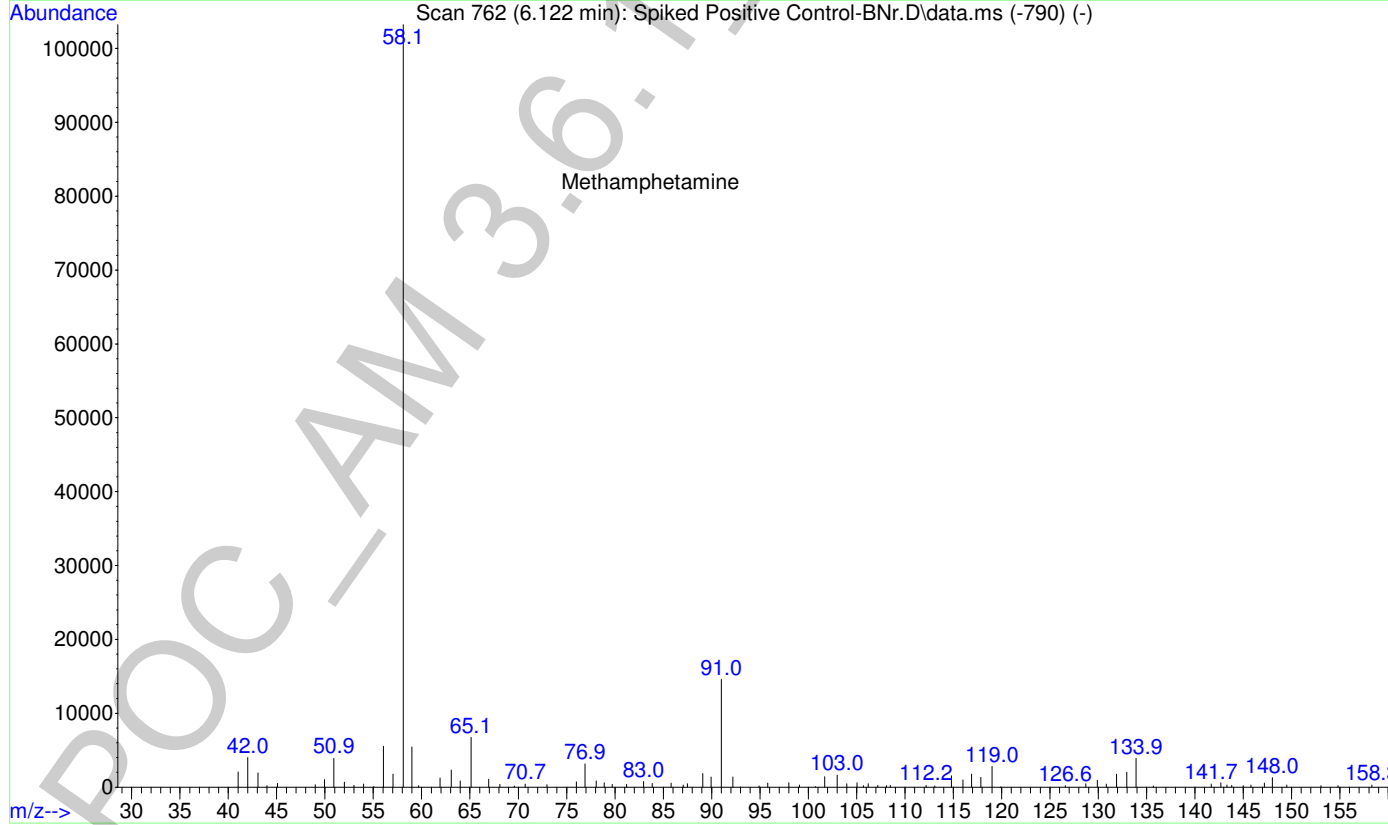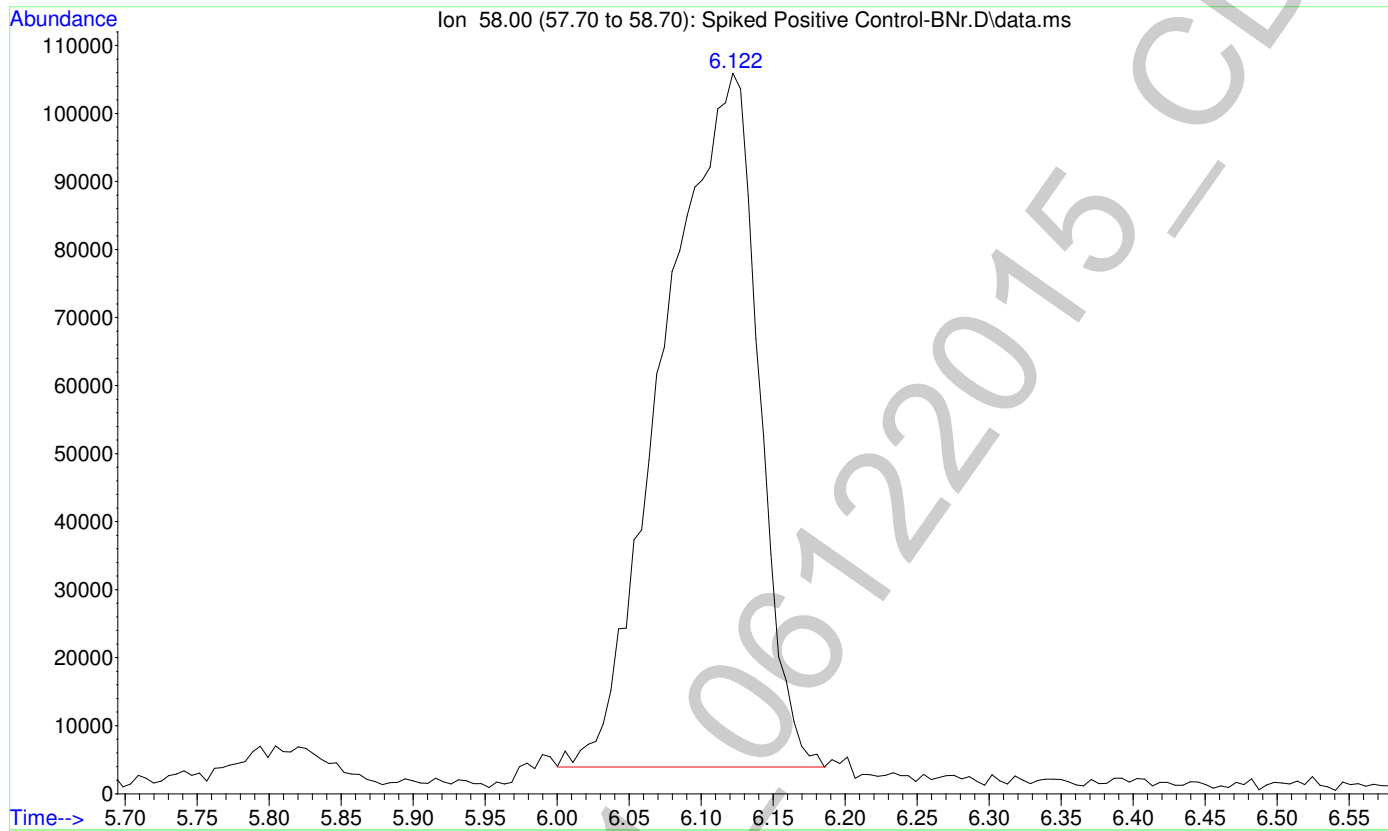



2

File : I:\Celena\061215\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 12 Jun 2015 15:45 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

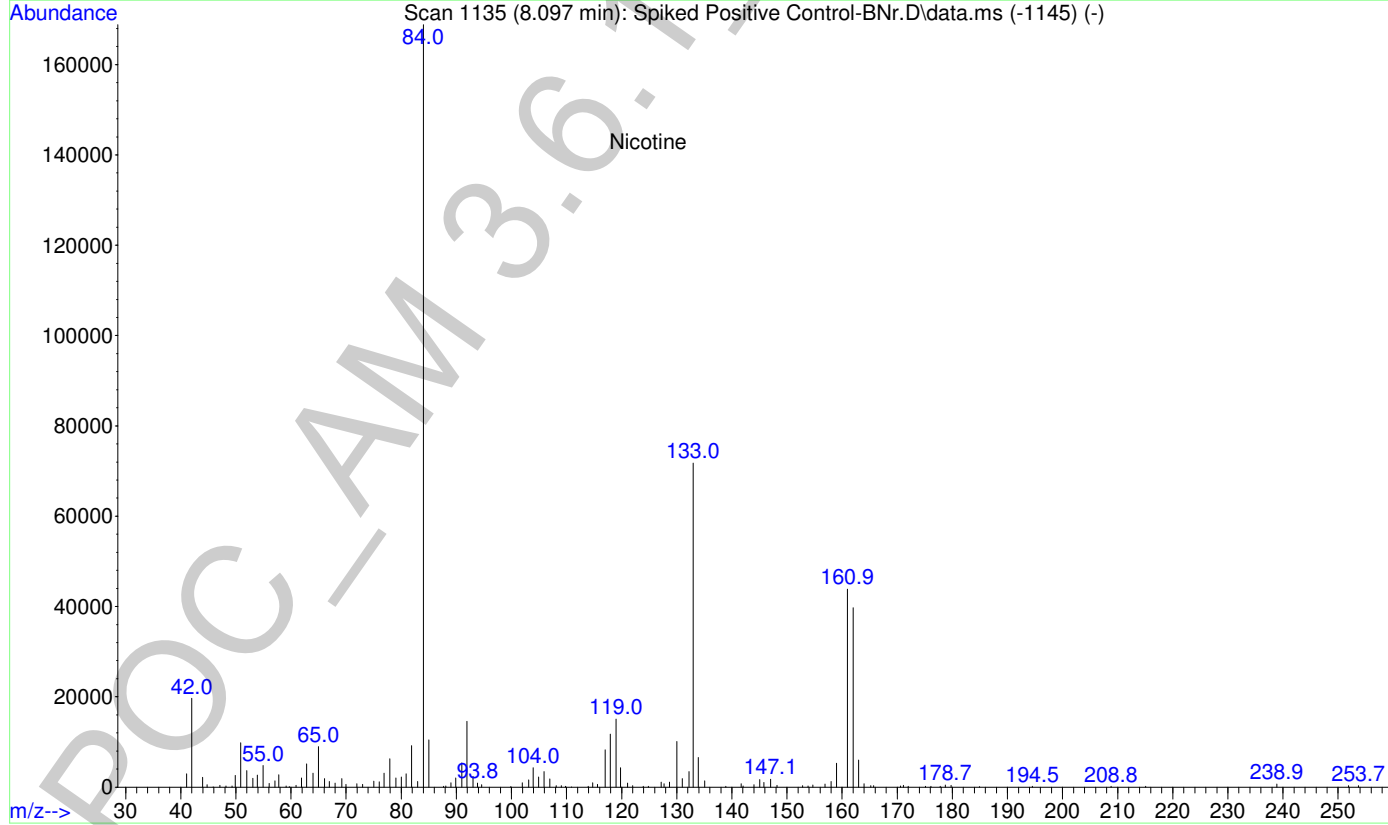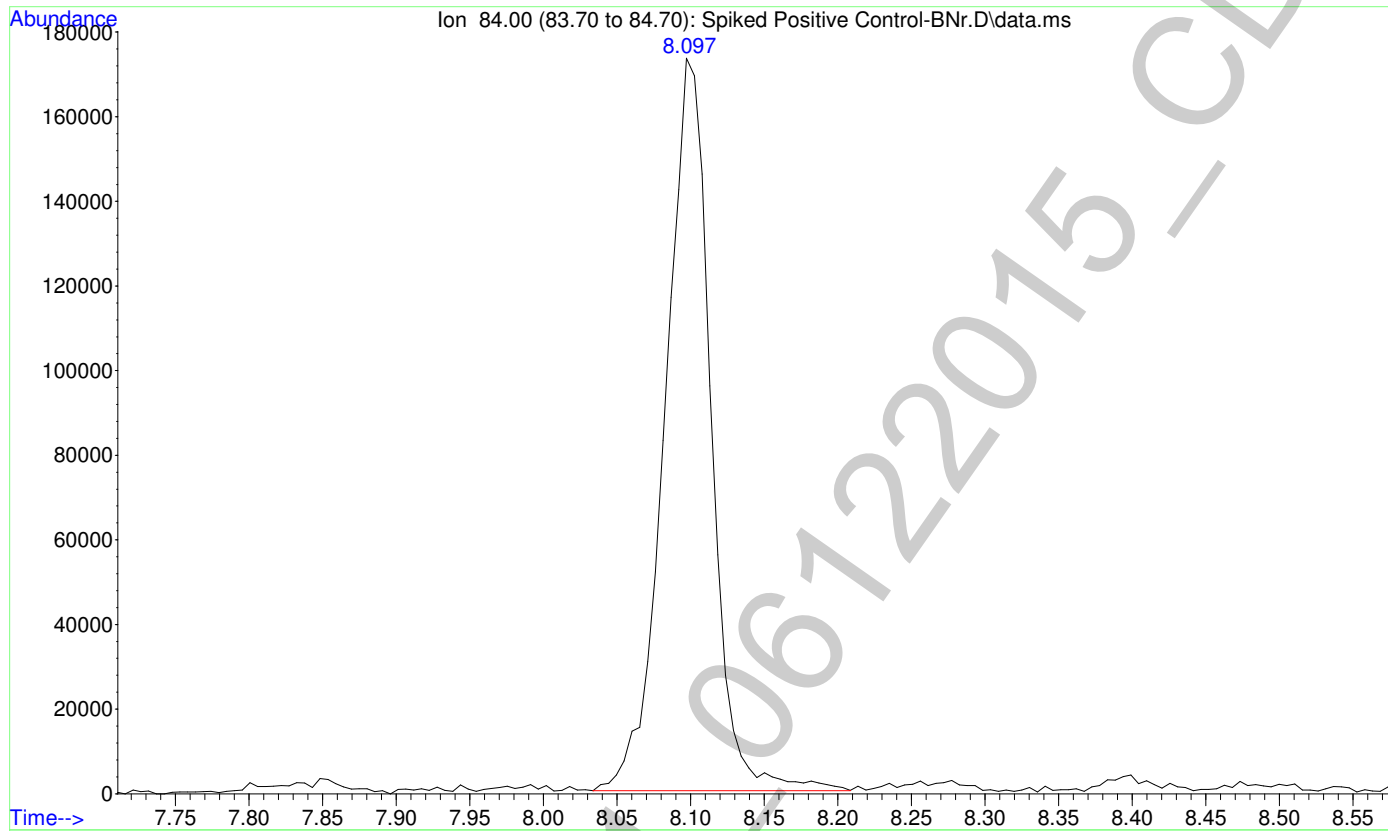



6

File : I:\Celena\061215\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 12 Jun 2015 15:45 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

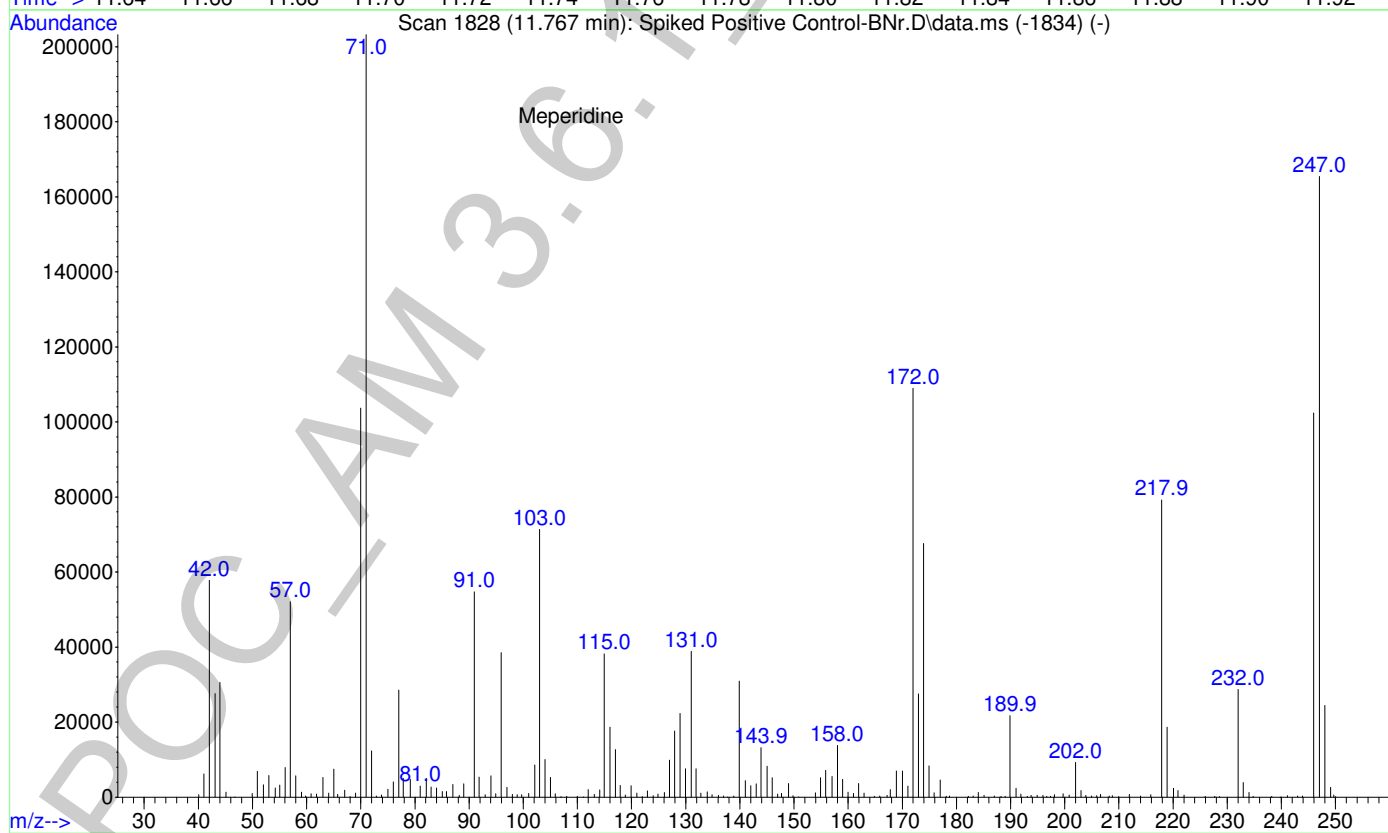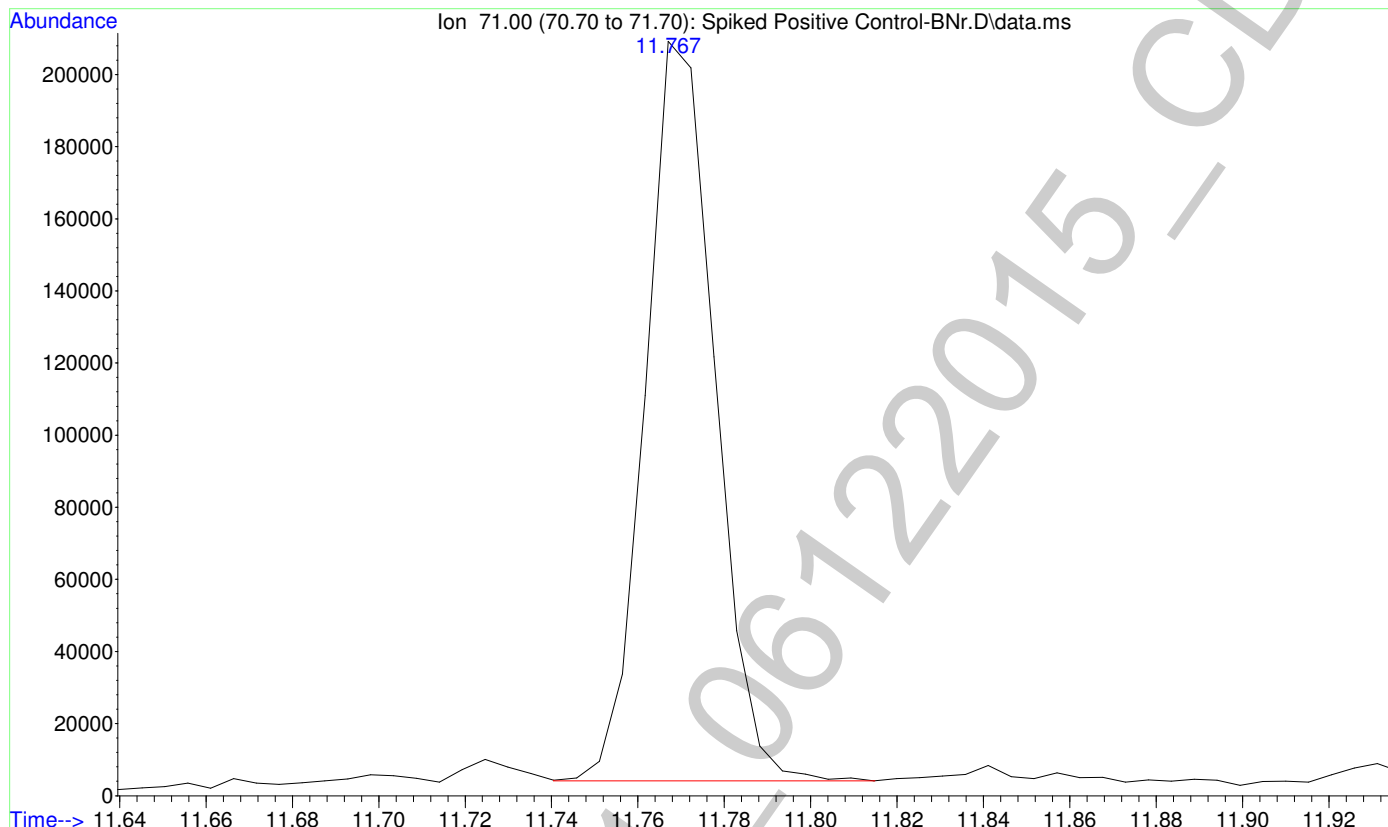



6

File : I:\Celena\061215\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 12 Jun 2015 15:45 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

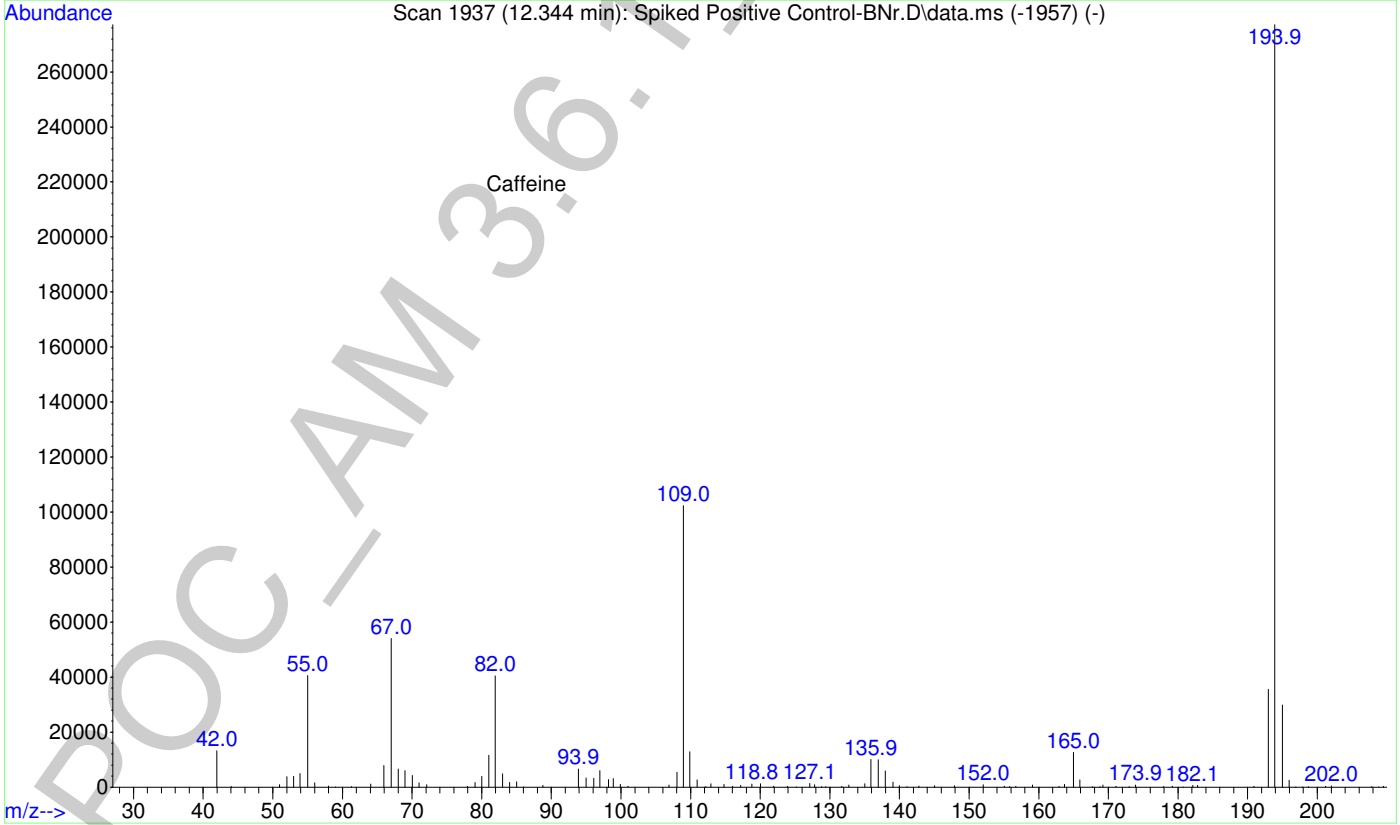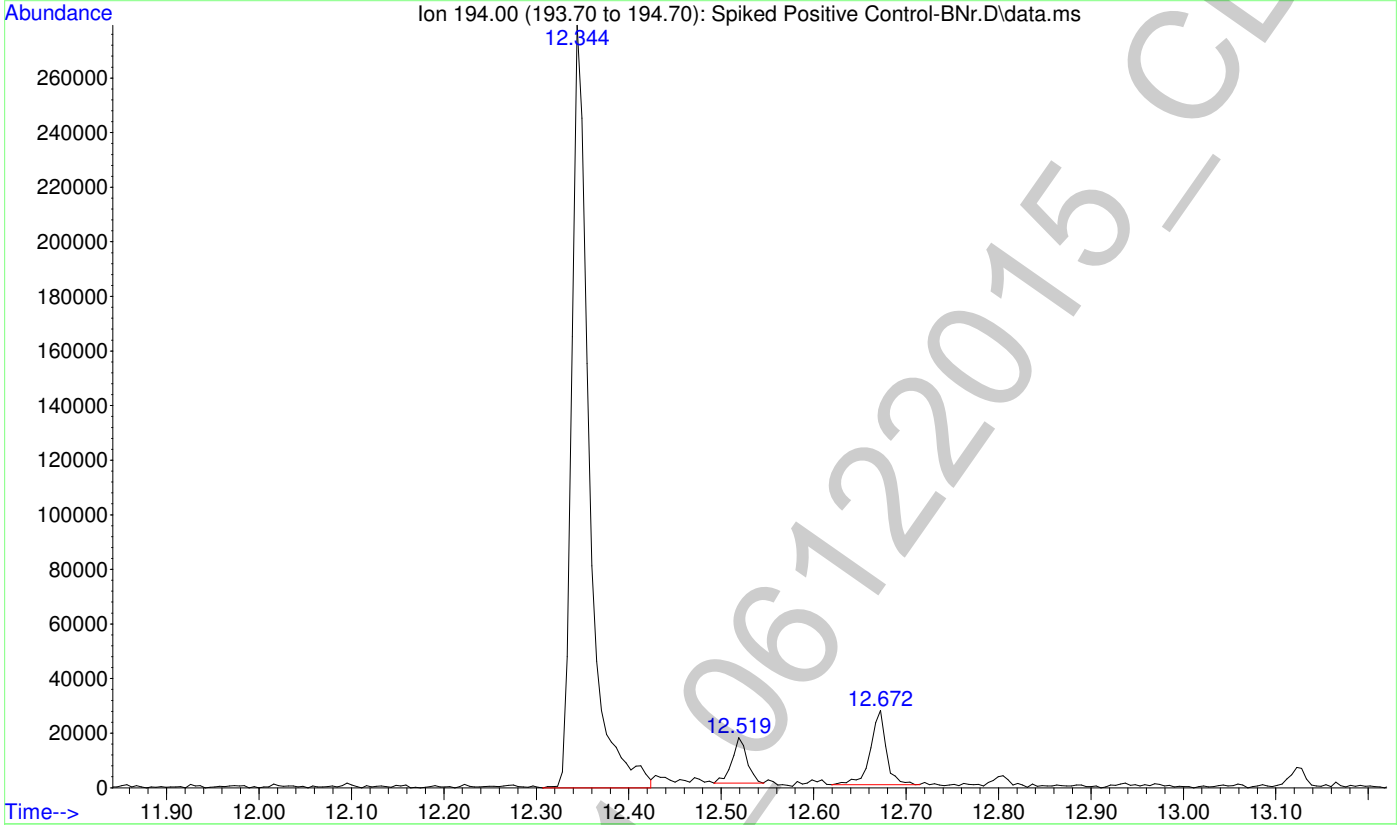



File : I:\Celena\061215\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 12 Jun 2015 15:45 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

2

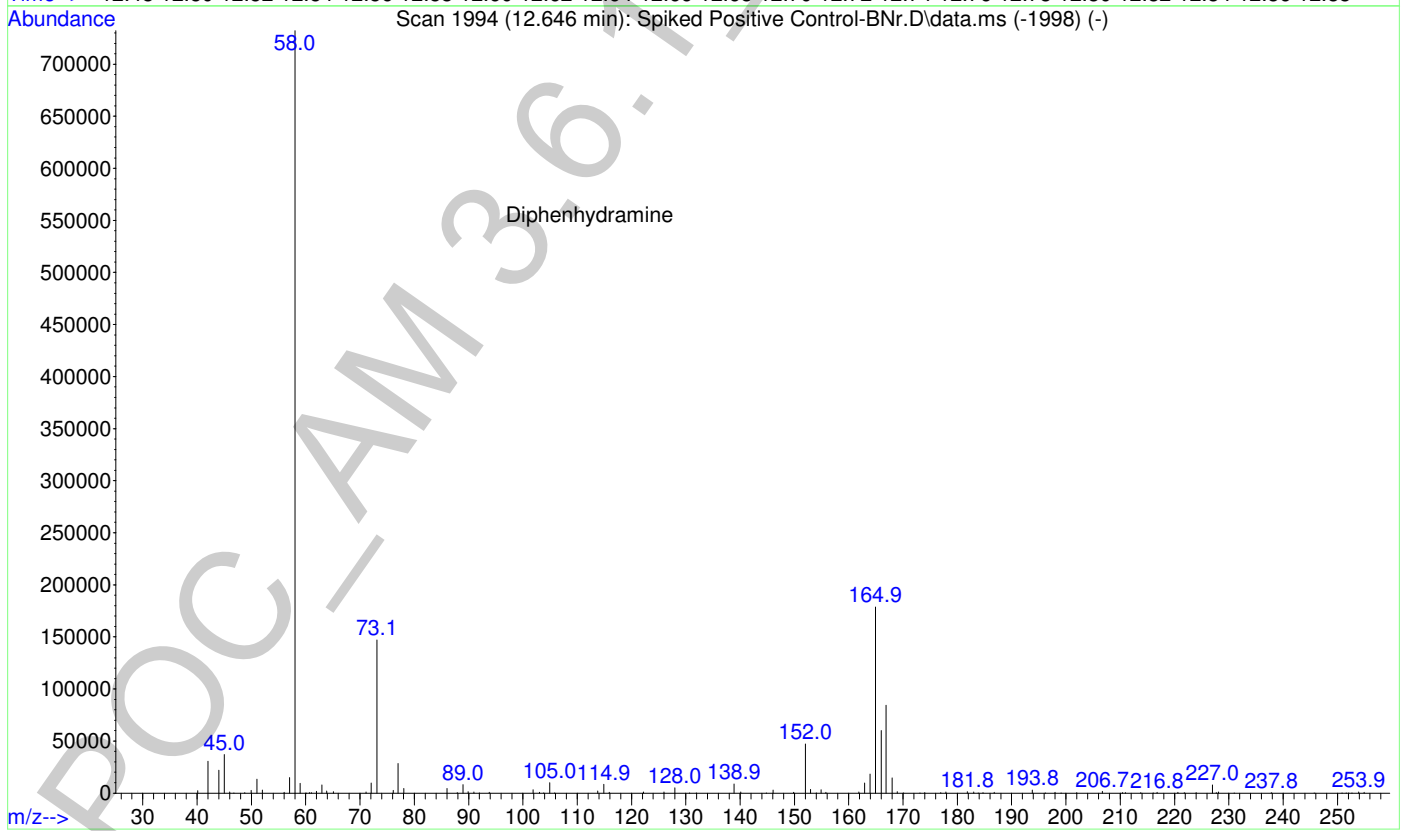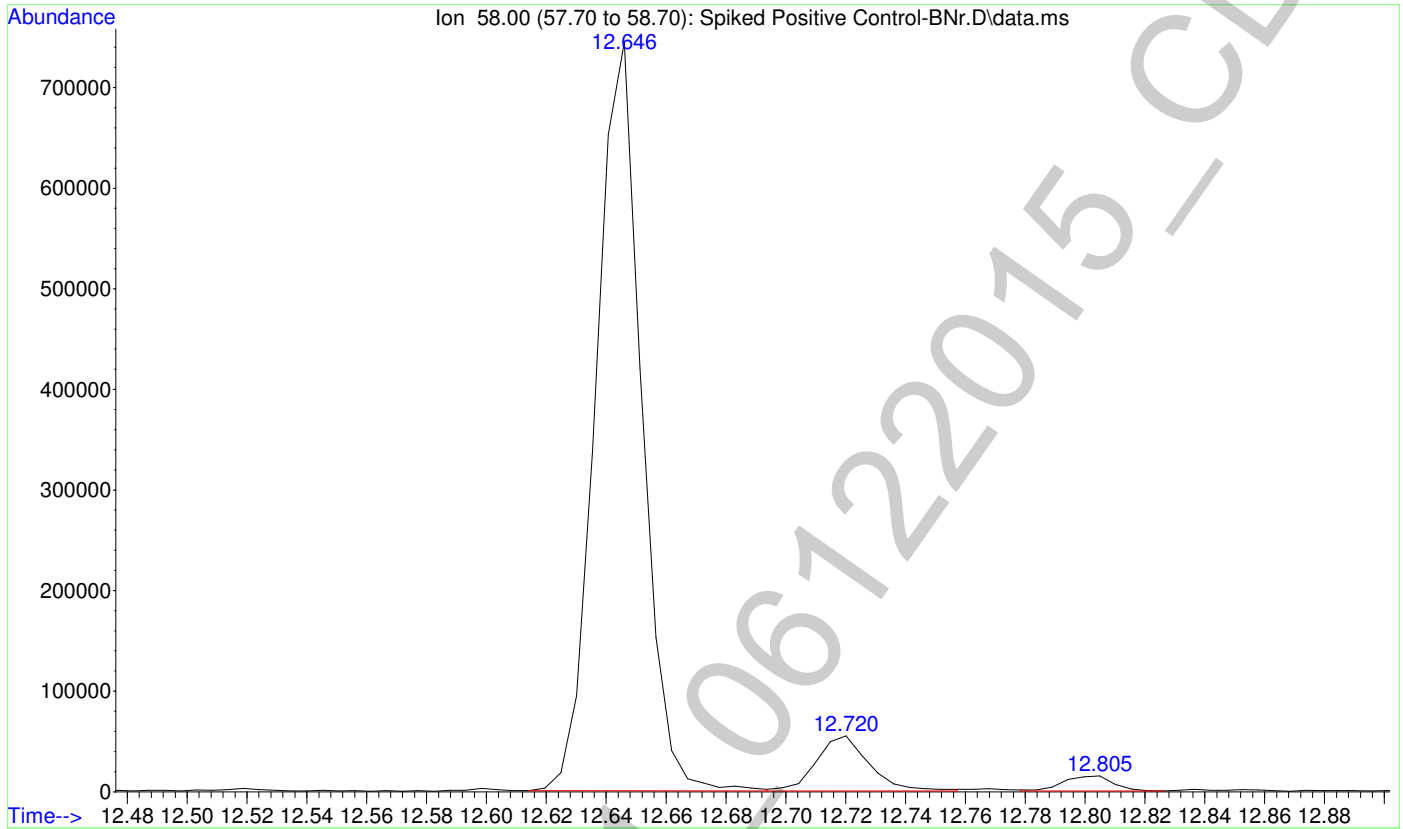



File : I:\Celena\061215\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 12 Jun 2015 15:45 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

2

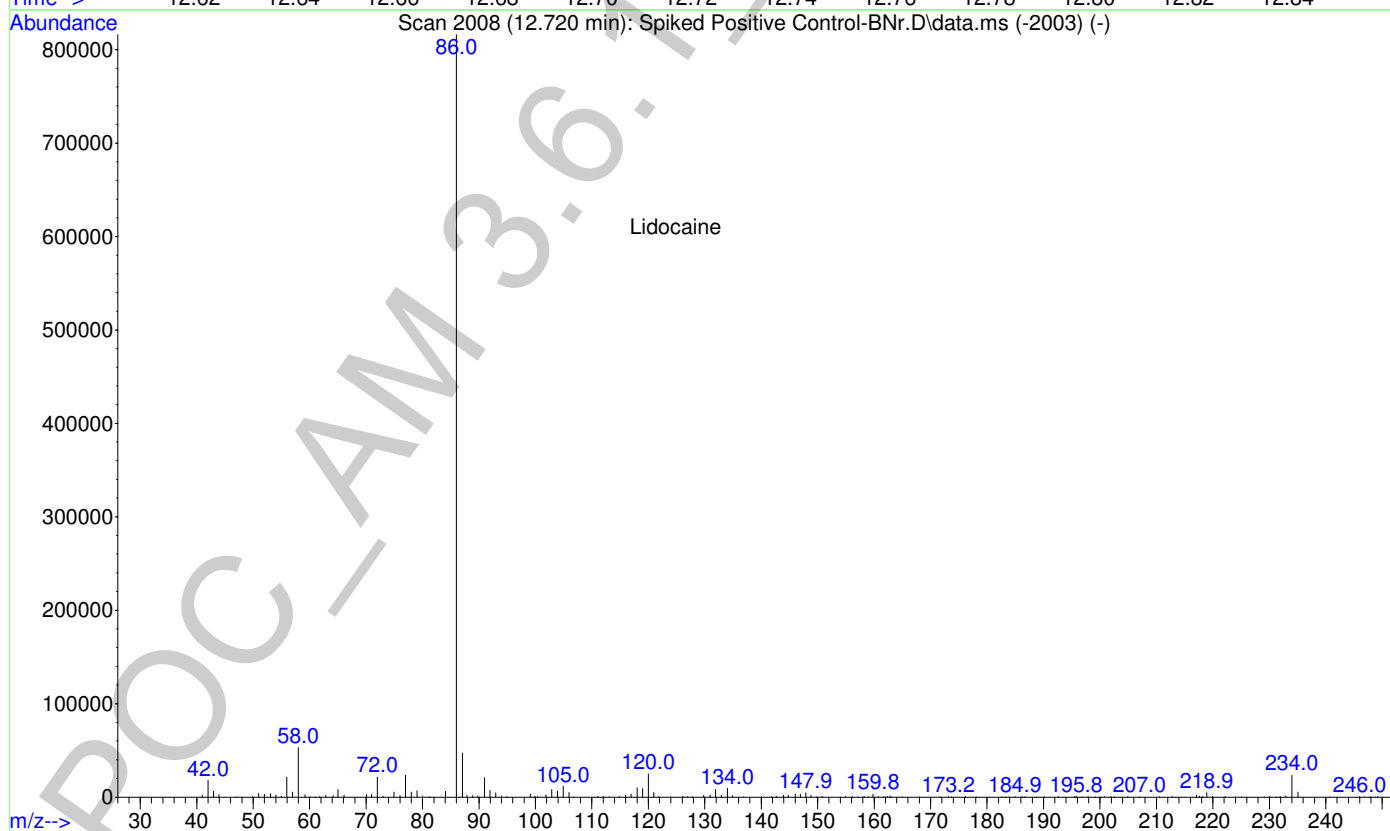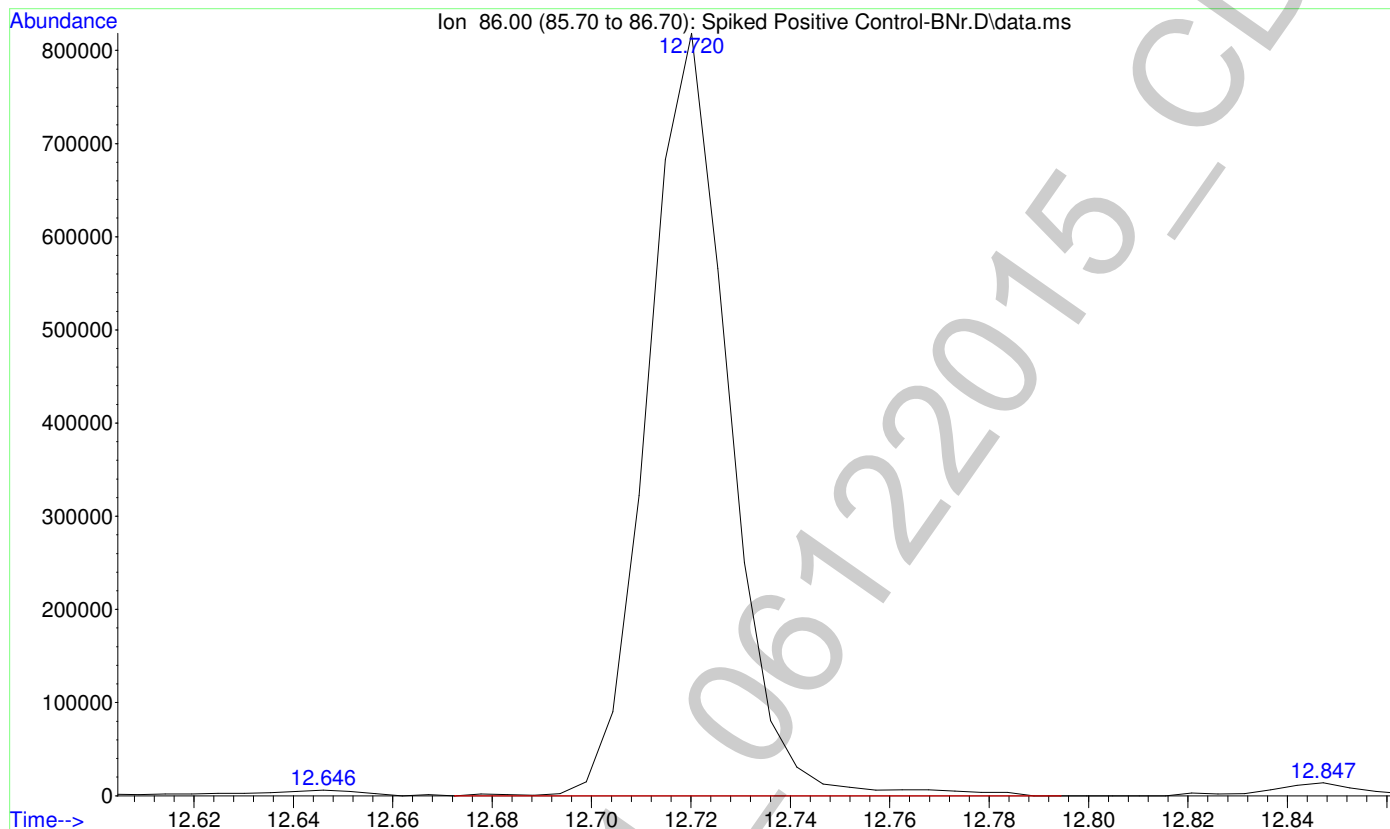



2

File : I:\Celena\061215\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 12 Jun 2015 15:45 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

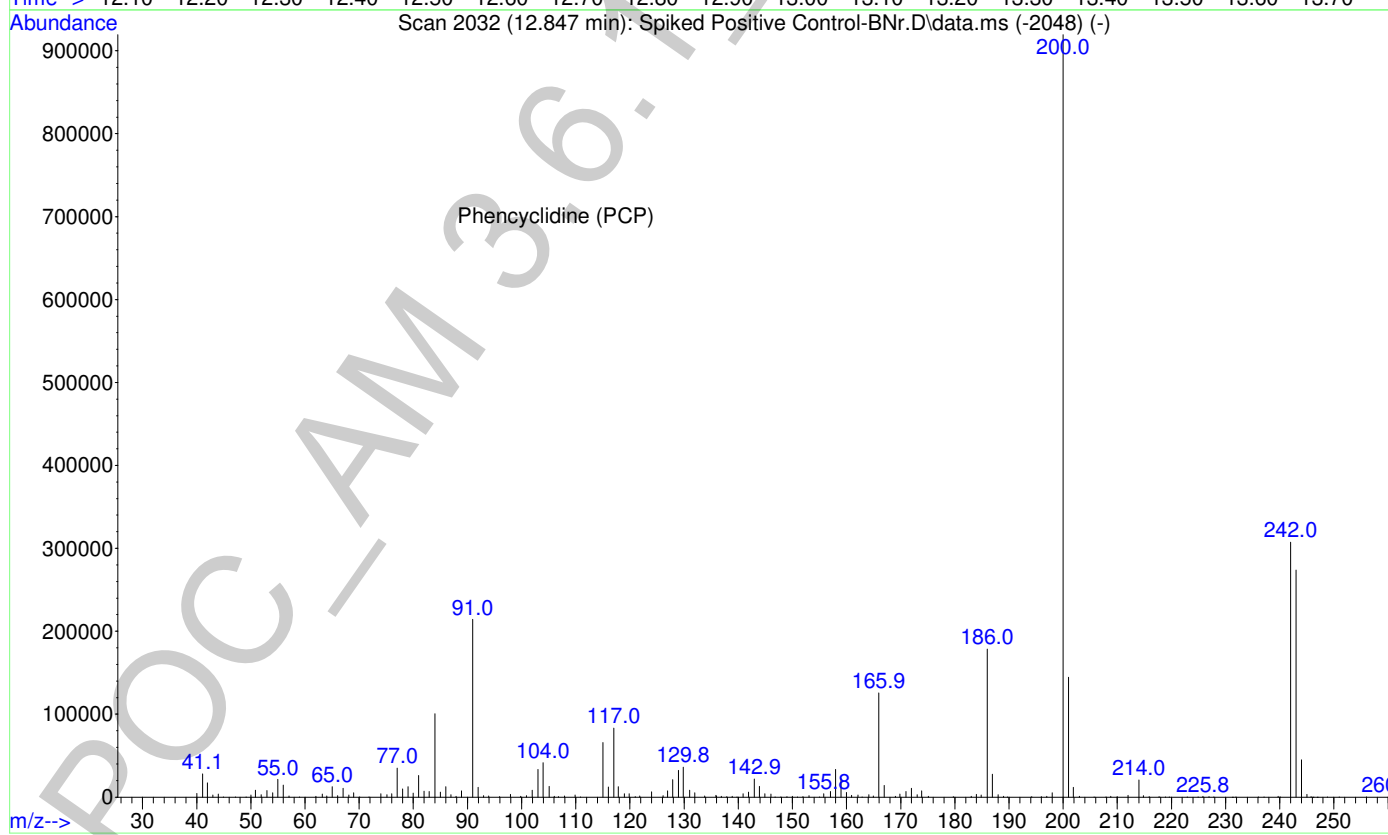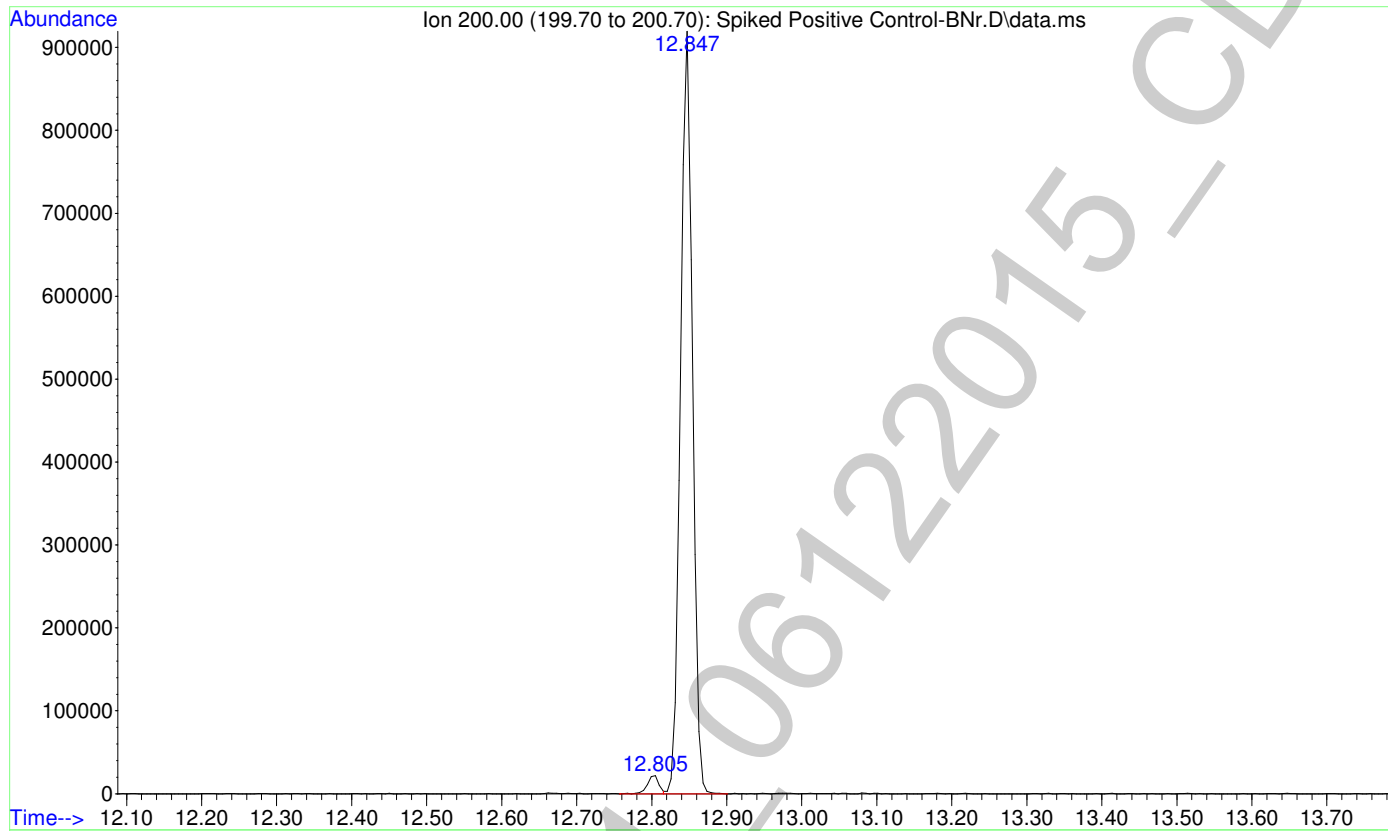



2

File : I:\Celena\061215\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 12 Jun 2015 15:45 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

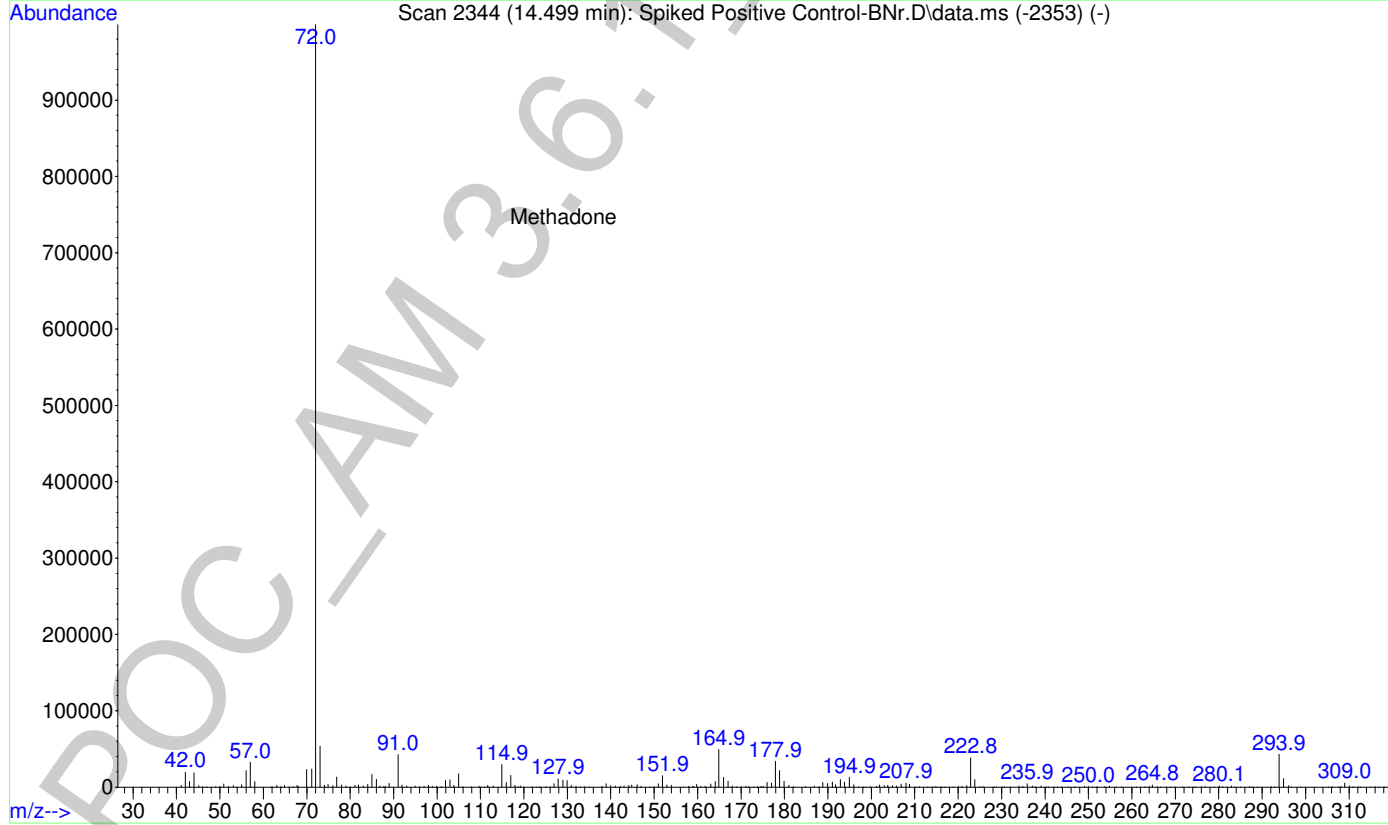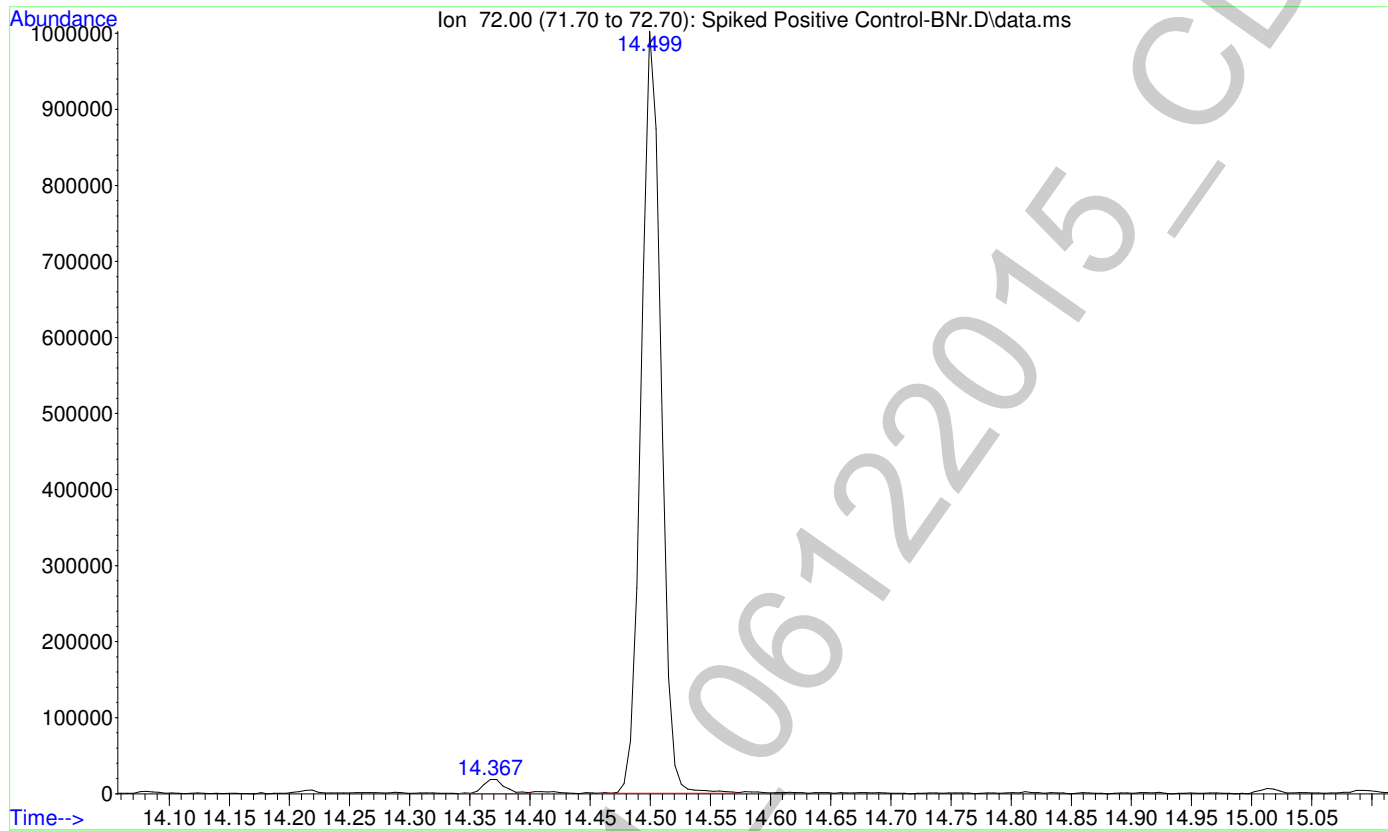



2

File : I:\Celena\061215\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 12 Jun 2015 15:45 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

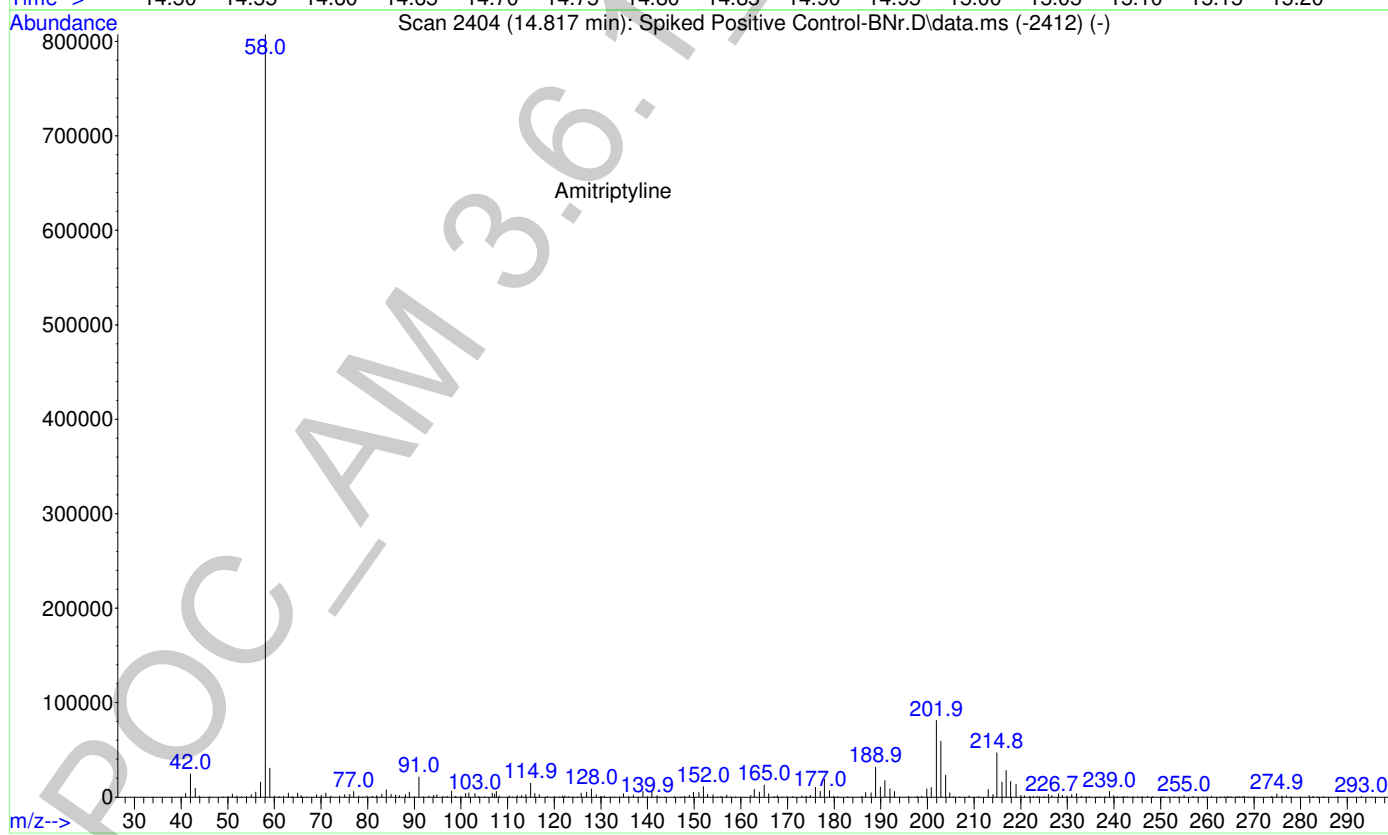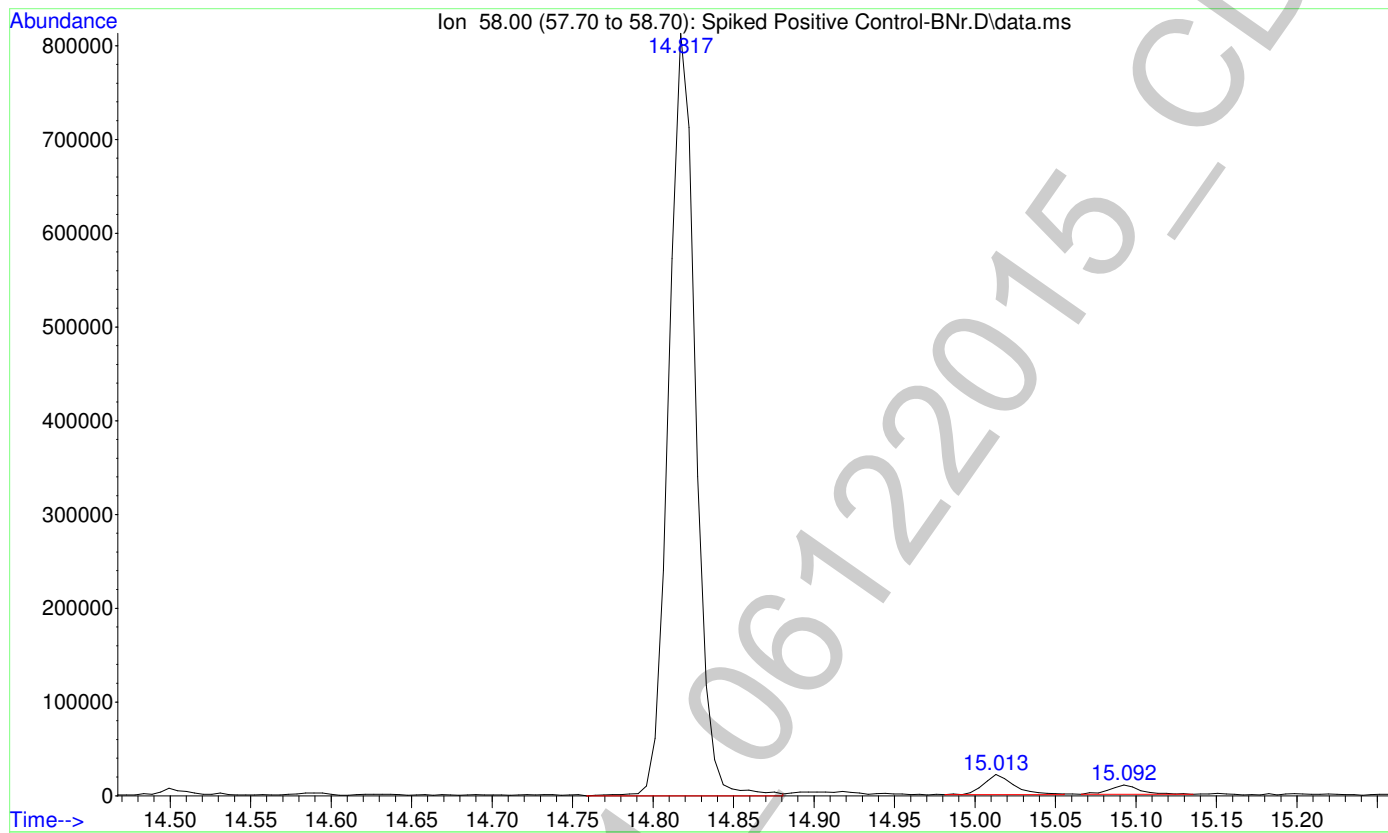

File : I:\Celena\061215\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 12 Jun 2015 15:45 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

2

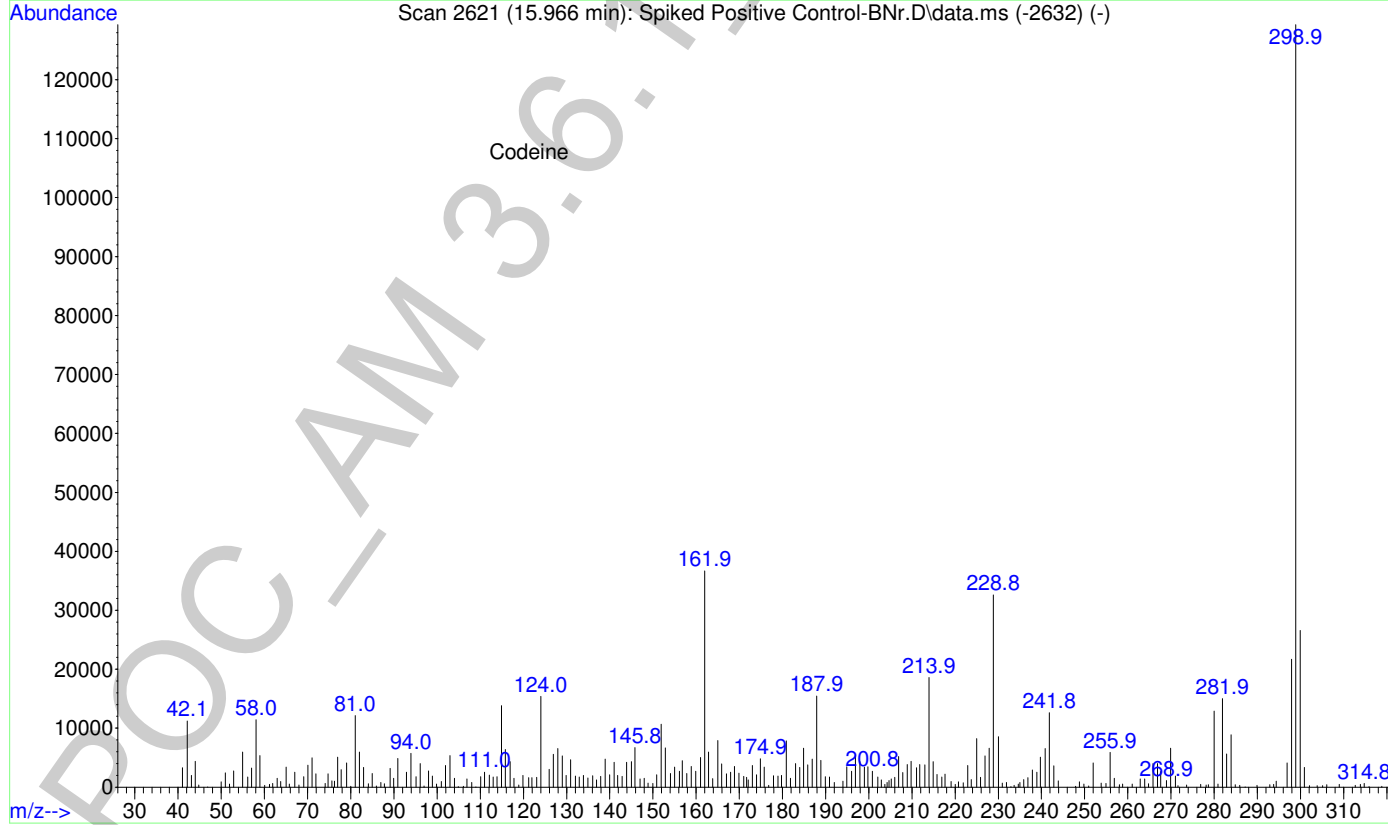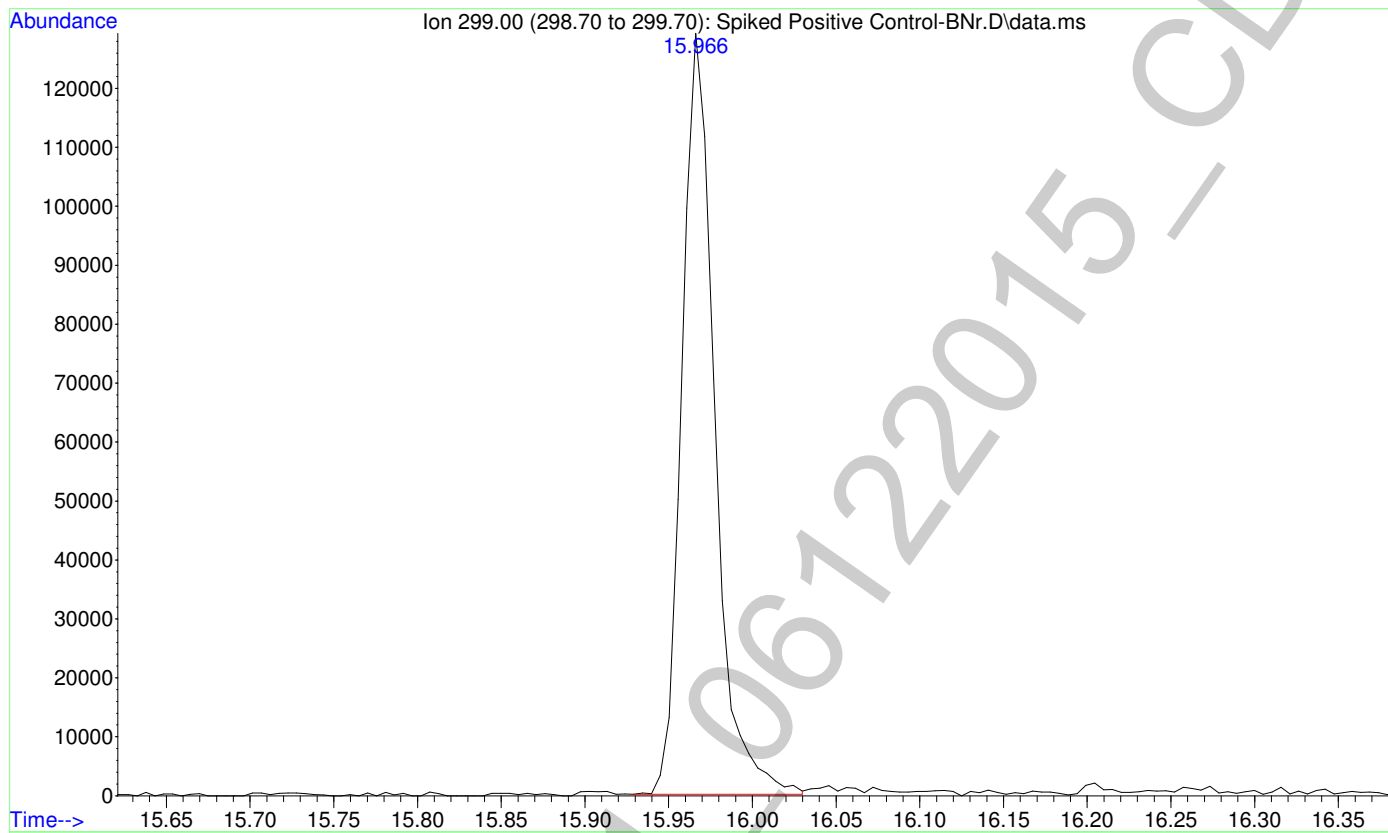

2

File : I:\Celena\061215\Spiked Positive Control-BNr.D
Operator : ISP\datastor
Acquired : 12 Jun 2015 15:45 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

