


Worklist: 607

<u>LAB_CASE</u>	<u>ITEM</u>	<u>TASK_ID</u>	<u>DESCRIPTION</u>	
M2015-0096	2	26280	3.6.1 Blood base neutral confirr	
M2015-0146	3	26932	3.6.1 Blood base neutral confirr	
M2015-0146	4	28935	3.6.1 Blood base neutral confirr	
M2015-0184	1	26877	3.6.1 Blood base neutral confirr	
M2015-0213	2	28499	3.6.1 Blood base neutral confirr	
M2015-0502	3	28753	3.6.1 Blood base neutral confirr	
M2015-0525	2	28636	3.6.1 Blood base neutral confirr	
P2015-0123	1	26277	3.6.1 Blood base neutral confirr	
P2015-0153	1	26397	3.6.1 Blood base neutral confirr	
P2015-0218	1	26852	3.6.1 Blood base neutral confirr	
P2015-0457	1	28247	3.6.1 Blood base neutral confirr	
P2015-0459	1	28268	3.6.1 Blood base neutral confirr	
P2015-0478	1	28341	3.6.1 Blood base neutral confirr	
P2015-0485	1	28414	3.6.1 Blood base neutral confirr	
P2015-0486	1	28418	3.6.1 Blood base neutral confirr	
P2015-0487	1	28424	3.6.1 Blood base neutral confirr	
P2015-0497	1	28467	3.6.1 Blood base neutral confirr	
P2015-0500	1	28512	3.6.1 Blood base neutral confirr	
P2015-0501	1	28515	3.6.1 Blood base neutral confirr	
P2015-0509	1	28608	3.6.1 Blood base neutral confirr	
P2015-0511	1	28630	3.6.1 Blood base neutral confirr	
P2015-0512	1	28633	3.6.1 Blood base neutral confirr	
P2015-0516	1	28668	3.6.1 Blood base neutral confirr	



Worklist: 607

<u>LAB CASE</u>	<u>ITEM</u>	<u>TASK ID</u>	<u>DESCRIPTION</u>
P2015-0520	1	28698	3.6.1 Blood base neutral confirr
P2015-0526	1	28761	3.6.1 Blood base neutral confirr



POC_AM 3.6.1_03062015_DND

CR 03/06/15.

simulate_sequence.log
Simulate Run Sequence Fri Mar 06 08:33:48 2015

Instrument Name: Major Mass Spec
Sequence File: C:\Users\ISPuser\Desktop\Sequences\DD-BNSB.sequence.xml
Comment: MassHunter sequence
Operator: 5LAB-C01\ISPuser
Data Path: D:\DATA\DND\2015\030615BN\
Method Path: D:\MassHunter\GCMS\1\methods\

Line	Type	Vials	DataFile	Sample Name
Acquisition Method: BNSB120510.M				
1)	Sample	100 ✓	Prerun Solvent Blank	Pre-run Solvent Blank
2)	Sample	1 ✓	Negative Control-BN	Negative Control -
...0130				
3)	Sample	2 ✓	Spiked Positive Control-BN	Positive Control
4)	Sample	99 ✓	prbLK2	Solvent Blank
Acquisition Method: GBT092509-Delta EMV.M				
5)	Sample	100 ✓	Prerun Solvent Blankr	Pre-run Solvent Blank
6)	Sample	1 ✓	Negative Control-BNr	Negative Control -
...0130				
7)	Sample	2 ✓	Spiked Positive Control-BNr	Positive Control
8)	Sample	99 ✓	prbLK2r	Solvent Blank
Acquisition Method: BNSB120510.M				
9)	Sample	98 ✓	P2015-0123-1-BNBLK	Lab No.: P2015-0123-1
10)	Sample	3 ✓	P2015-0123-1-BN	Lab No.: P2015-0123-1
11)	Sample	97 ✓	P2015-0153-1-BNBLK	Lab No.: P2015-0153-1
12)	Sample	4 ✓	P2015-0153-1-BN	Lab No.: P2015-0153-1
13)	Sample	96 ✓	P2015-0218-1-BNBLK	Lab No.: P2015-0218-1
14)	Sample	5 ✓	P2015-0218-1-BN	Lab No.: P2015-0218-1
15)	Sample	95 ✓	P2015-0457-1-BNBLK	Lab No.: P2015-0457-1
16)	Sample	6 ✓	P2015-0457-1-BN	Lab No.: P2015-0457-1
17)	Sample	94 ✓	P2015-0459-1-BNBLK	Lab No.: P2015-0459-1
18)	Sample	7 ✓	P2015-0459-1-BN	Lab No.: P2015-0459-1
19)	Sample	93 ✓	P2015-0478-1-BNBLK	Lab No.: P2015-0478-1
20)	Sample	8 ✓	P2015-0478-1-BN	Lab No.: P2015-0478-1
21)	Sample	92 ✓	P2015-0485-1-BNBLK	Lab No.: P2015-0485-1
22)	Sample	9 ✓	P2015-0485-1-BN	Lab No.: P2015-0485-1
23)	Sample	91 ✓	P2015-0486-1-BNBLK	Lab No.: P2015-0486-1
24)	Sample	10 ✓	P2015-0486-1-BN	Lab No.: P2015-0486-1
Acquisition Method: GBT092509-Delta EMV.M				
25)	Sample	98 ✓	P2015-0123-1-BNBLKCr	Lab No.: P2015-0123-1
26)	Sample	3 ✓	P2015-0123-1-BNr	Lab No.: P2015-0123-1
27)	Sample	97 ✓	P2015-0153-1-BNBLKCr	Lab No.: P2015-0153-1
28)	Sample	4 ✓	P2015-0153-1-BNr	Lab No.: P2015-0153-1
29)	Sample	96 ✓	P2015-0218-1-BNBLKCr	Lab No.: P2015-0218-1
30)	Sample	5 ✓	P2015-0218-1-BNr	Lab No.: P2015-0218-1
31)	Sample	95 ✓	P2015-0457-1-BNBLKCr	Lab No.: P2015-0457-1
32)	Sample	6 ✓	P2015-0457-1-BNr	Lab No.: P2015-0457-1
33)	Sample	94 ✓	P2015-0459-1-BNBLKCr	Lab No.: P2015-0459-1
34)	Sample	7 ✓	P2015-0459-1-BNr	Lab No.: P2015-0459-1
35)	Sample	93 ✓	P2015-0478-1-BNBLKCr	Lab No.: P2015-0478-1
36)	Sample	8 ✓	P2015-0478-1-BNr	Lab No.: P2015-0478-1
37)	Sample	92 ✓	P2015-0485-1-BNBLKCr	Lab No.: P2015-0485-1
38)	Sample	9 ✓	P2015-0485-1-BNr	Lab No.: P2015-0485-1
39)	Sample	91 ✓	P2015-0486-1-BNBLKCr	Lab No.: P2015-0486-1
40)	Sample	10 ✓	P2015-0486-1-BNr	Lab No.: P2015-0486-1
Acquisition Method: BNSB120510.M				
41)	Sample	90 ✓	P2015-0487-1-BNBLK	Lab No.: P2015-0487-1
42)	Sample	11 ✓	P2015-0487-1-BN	Lab No.: P2015-0487-1
43)	Sample	89 ✓	P2015-0497-1-BNBLK	Lab No.: P2015-0497-1
44)	Sample	12 ✓	P2015-0497-1-BN	Lab No.: P2015-0497-1

ge 03/06/15.

simulate_sequence.log

45) Sample	88 ✓	P2015-0500-1-BNBLK	Lab No.:	P2015-0500-1
46) Sample	13 ✓	P2015-0500-1-BN	Lab No.:	P2015-0500-1
47) Sample	87 ✓	P2015-0501-1-BNBLK	Lab No.:	P2015-0501-1
48) Sample	14 ✓	P2015-0501-1-BN	Lab No.:	P2015-0501-1
49) Sample	86 ✓	P2015-0509-1-BNBLK	Lab No.:	P2015-0509-1
50) Sample	15 ✓	P2015-0509-1-BN	Lab No.:	P2015-0509-1

Acquisition Method: GBT092509-Delta EMV.M

51) Sample	90 ✓	P2015-0487-1-BNBLKr	Lab No.:	P2015-0487-1
52) Sample	11 ✓	P2015-0487-1-BNr	Lab No.:	P2015-0487-1
53) Sample	89 ✓	P2015-0497-1-BNBLKr	Lab No.:	P2015-0497-1
54) Sample	12 ✓	P2015-0497-1-BNr	Lab No.:	P2015-0497-1
55) Sample	88 ✓	P2015-0500-1-BNBLKr	Lab No.:	P2015-0500-1
56) Sample	13 ✓	P2015-0500-1-BNr	Lab No.:	P2015-0500-1
57) Sample	87 ✓	P2015-0501-1-BNBLKr	Lab No.:	P2015-0501-1
58) Sample	14 ✓	P2015-0501-1-BNr	Lab No.:	P2015-0501-1
59) Sample	86 ✓	P2015-0509-1-BNBLKr	Lab No.:	P2015-0509-1
60) Sample	15 ✓	P2015-0509-1-BNr	Lab No.:	P2015-0509-1

Acquisition Method: BNSB120510.M

61) Sample	85 ✓	P2015-0511-1-BNBLK	Lab No.:	P2015-0511-1
62) Sample	16 ✓	P2015-0511-1-BN	Lab No.:	P2015-0511-1
63) Sample	84 ✓	P2015-0512-1-BNBLK	Lab No.:	P2015-0512-1
64) Sample	17 ✓	P2015-0512-1-BN	Lab No.:	P2015-0512-1
65) Sample	83 ✓	P2015-0516-1-BNBLK	Lab No.:	P2015-0516-1
66) Sample	18 ✓	P2015-0516-1-BN	Lab No.:	P2015-0516-1
67) Sample	82 ✓	P2015-0520-1-BNBLK	Lab No.:	P2015-0520-1
68) Sample	19 ✓	P2015-0520-1-BN	Lab No.:	P2015-0520-1
69) Sample	81 ✓	P2015-0526-1-BNBLK	Lab No.:	P2015-0526-1
70) Sample	20 ✓	P2015-0526-1-BN	Lab No.:	P2015-0526-1

Acquisition Method: GBT092509-Delta EMV.M

71) Sample	85 ✓	P2015-0511-1-BNBLKr	Lab No.:	P2015-0511-1
72) Sample	16 ✓	P2015-0511-1-BNr	Lab No.:	P2015-0511-1
73) Sample	84 ✓	P2015-0512-1-BNBLKr	Lab No.:	P2015-0512-1
74) Sample	17 ✓	P2015-0512-1-BNr	Lab No.:	P2015-0512-1
75) Sample	83 ✓	P2015-0516-1-BNBLKr	Lab No.:	P2015-0516-1
76) Sample	18 ✓	P2015-0516-1-BNr	Lab No.:	P2015-0516-1
77) Sample	82 ✓	P2015-0520-1-BNBLKr	Lab No.:	P2015-0520-1
78) Sample	19 ✓	P2015-0520-1-BNr	Lab No.:	P2015-0520-1
79) Sample	81 ✓	P2015-0526-1-BNBLKr	Lab No.:	P2015-0526-1
80) Sample	20 ✓	P2015-0526-1-BNr	Lab No.:	P2015-0526-1

Acquisition Method: BNSB120510.M

81) Sample	80 ✓	M2015-0096-2-BNBLK	Lab No.:	M2015-0096-2
82) Sample	21 ✓	M2015-0096-2-BN	Lab No.:	M2015-0096-2
83) Sample	79 ✓	M2015-0146-3-BNBLK	Lab No.:	M2015-0146-3
84) Sample	22 ✓	M2015-0146-3-BN	Lab No.:	M2015-0146-3
85) Sample	78 ✓	M2015-0146-4-BNBLK	Lab No.:	M2015-0146-4
86) Sample	23 ✓	M2015-0146-4-BN	Lab No.:	M2015-0146-4
87) Sample	77 ✓	M2015-0184-1-BNBLK	Lab No.:	M2015-0184-1
88) Sample	24 ✓	M2015-0184-1-BN	Lab No.:	M2015-0184-1
89) Sample	76 ✓	M2015-0213-2-BNBLK	Lab No.:	M2015-0213-2
90) Sample	25 ✓	M2015-0213-2-BN	Lab No.:	M2015-0213-2

Acquisition Method: GBT092509-Delta EMV.M

91) Sample	80 ✓	M2015-0096-2-BNBLKr	Lab No.:	M2015-0096-2
92) Sample	21 ✓	M2015-0096-2-BNr	Lab No.:	M2015-0096-2
93) Sample	79 ✓	M2015-0146-3-BNBLKr	Lab No.:	M2015-0146-3
94) Sample	22 ✓	M2015-0146-3-BNr	Lab No.:	M2015-0146-3
95) Sample	78 ✓	M2015-0146-4-BNBLKr	Lab No.:	M2015-0146-4
96) Sample	23 ✓	M2015-0146-4-BNr	Lab No.:	M2015-0146-4
97) Sample	77 ✓	M2015-0184-1-BNBLKr	Lab No.:	M2015-0184-1
98) Sample	24 ✓	M2015-0184-1-BNr	Lab No.:	M2015-0184-1
99) Sample	76 ✓	M2015-0213-2-BNBLKr	Lab No.:	M2015-0213-2
100) Sample	25 ✓	M2015-0213-2-BNr	Lab No.:	M2015-0213-2

Acquisition Method: BNSB120510.M

02/03/06/15

simulate_sequence.log
101) Sample 75 ✓ M2015-0502-3-BNBLK Lab No.: M2015-0502-3
102) Sample 26 ✓ M2015-0502-3-BN Lab No.: M2015-0502-3
103) Sample 74 ✓ M2015-0525-2-BNBLK Lab No.: M2015-0525-2
104) Sample 27 ✓ M2015-0525-2-BN Lab No.: M2015-0525-2

Acquisition Method: GBT092509-Delta EMV.M
105) Sample 75 ✓ M2015-0502-3-BNBLKr Lab No.: M2015-0502-3
106) Sample 26 ✓ M2015-0502-3-BNr Lab No.: M2015-0502-3
107) Sample 74 ✓ M2015-0525-2-BNBLKr Lab No.: M2015-0525-2
108) Sample 27 ✓ M2015-0525-2-BNr Lab No.: M2015-0525-2

Acquisition Method: BNSB120510.M
109) Sample 73 ✓ POSTBLK BLK

Acquisition Method: GBT092509-Delta EMV.M
110) Sample 72 ✓ AFTER BLK
megabytes Needed: 2279 Space on drive D: 312793
Sequence Verification Done!

POC_AM 3.6.1_03062015



Analytical Method 3.6.1 & 3.6.7 QA Check List

Run Start Date: 03/06/15

Analyst: DND

(Short GC/MS temperature program)

Positive Control Compound List



- Methamphetamine
- Nicotine
- Meperidine
- Caffeine
- Diphenhydramine
- Lidocaine
- PCP
- Methadone
- Amitriptyline
- Codeine
- Trazodone

Internal Standards



- Benzphetamine
- Papaverine

Optional back extraction **not** performed.
Samples reconstituted in methanol.

File :C:\gcms\1\data\Blood\030615BN\Prerun Solvent Blank.D
Operator : 5LAB-C01\ISPuser
Acquired : 06 Mar 2015 08:47 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Pre-run Solvent Blank
Misc Info : Chloroform
Vial Number: 100

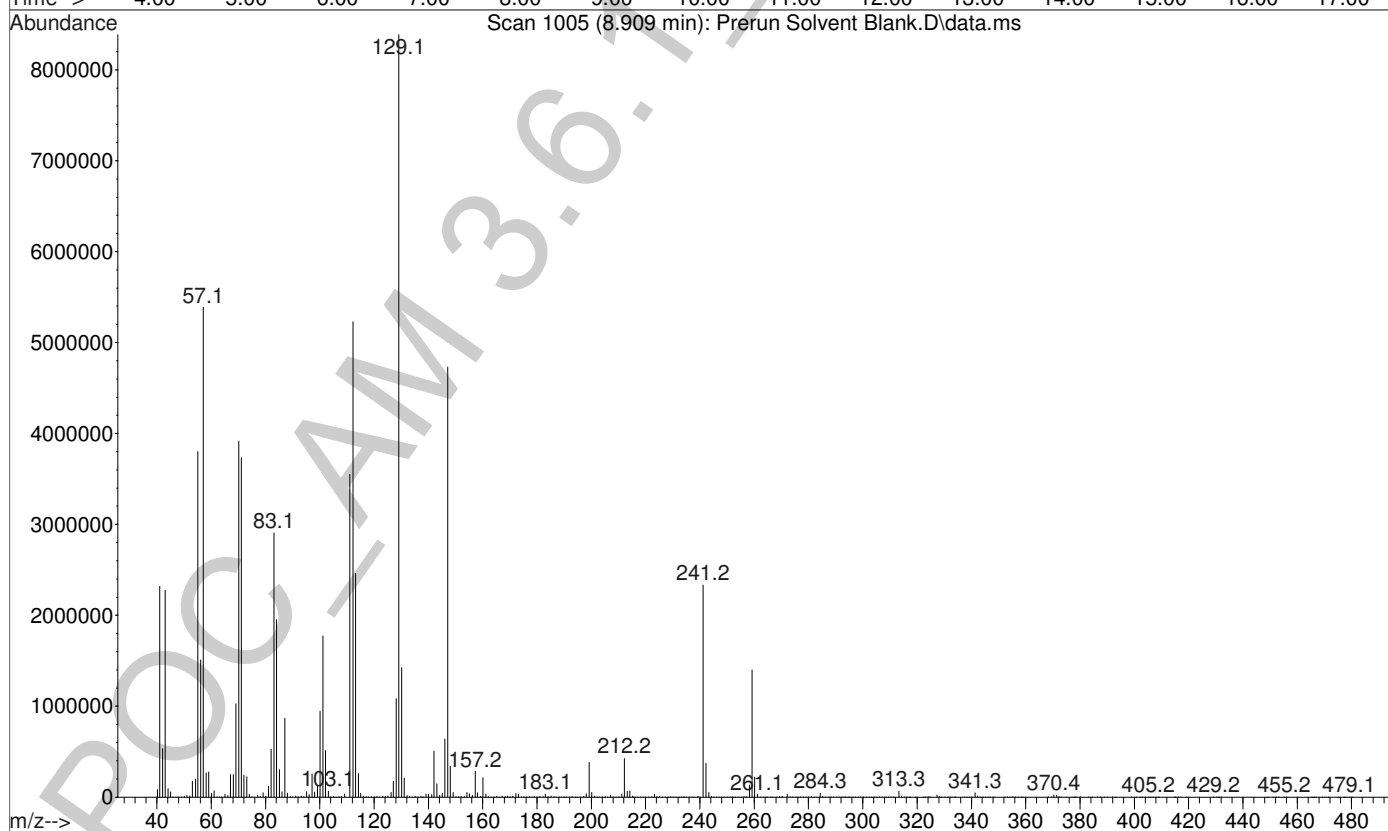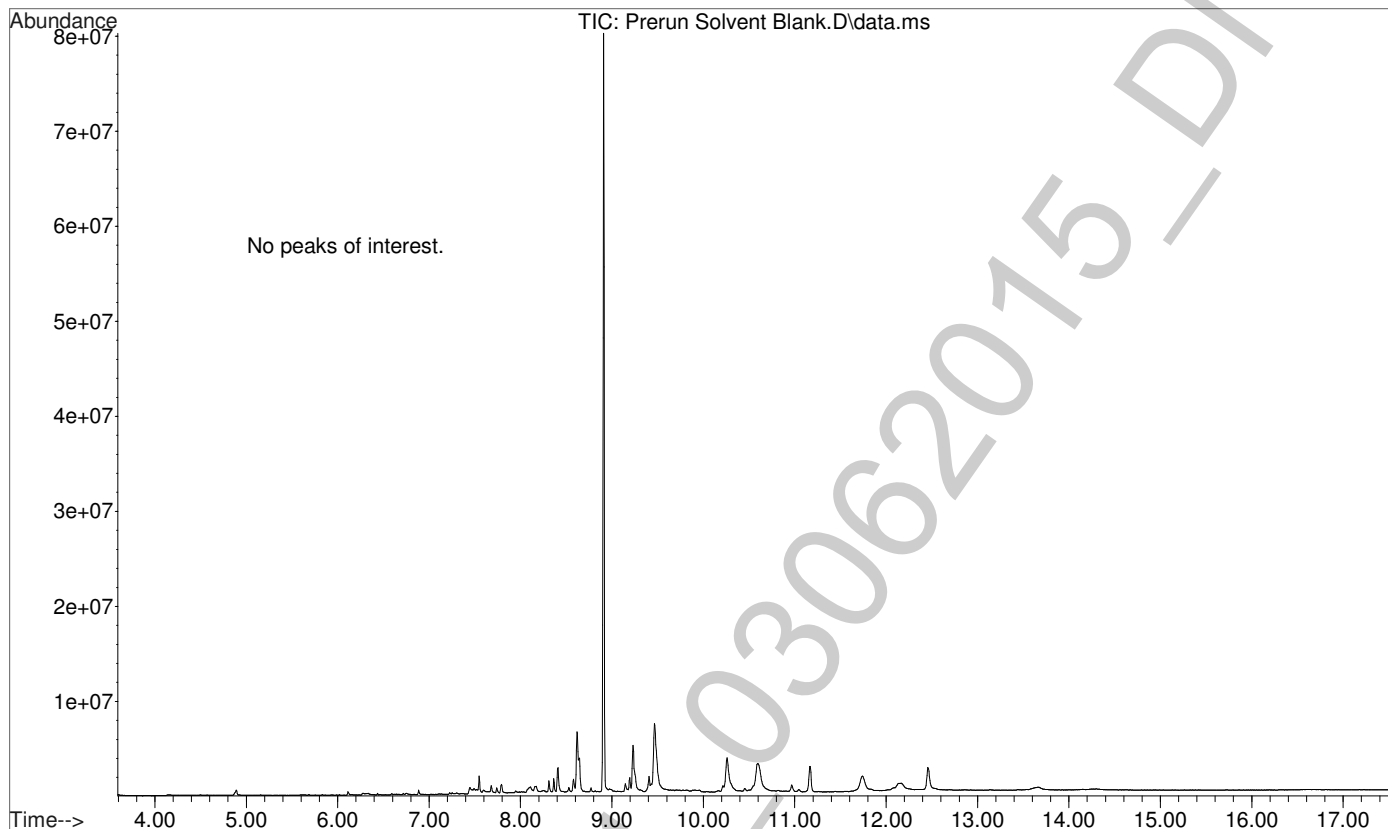


Library Searched : C:\Database\DD2012.L
Quality : 95
ID : 2-Ethylhexyl hydrogen adipate

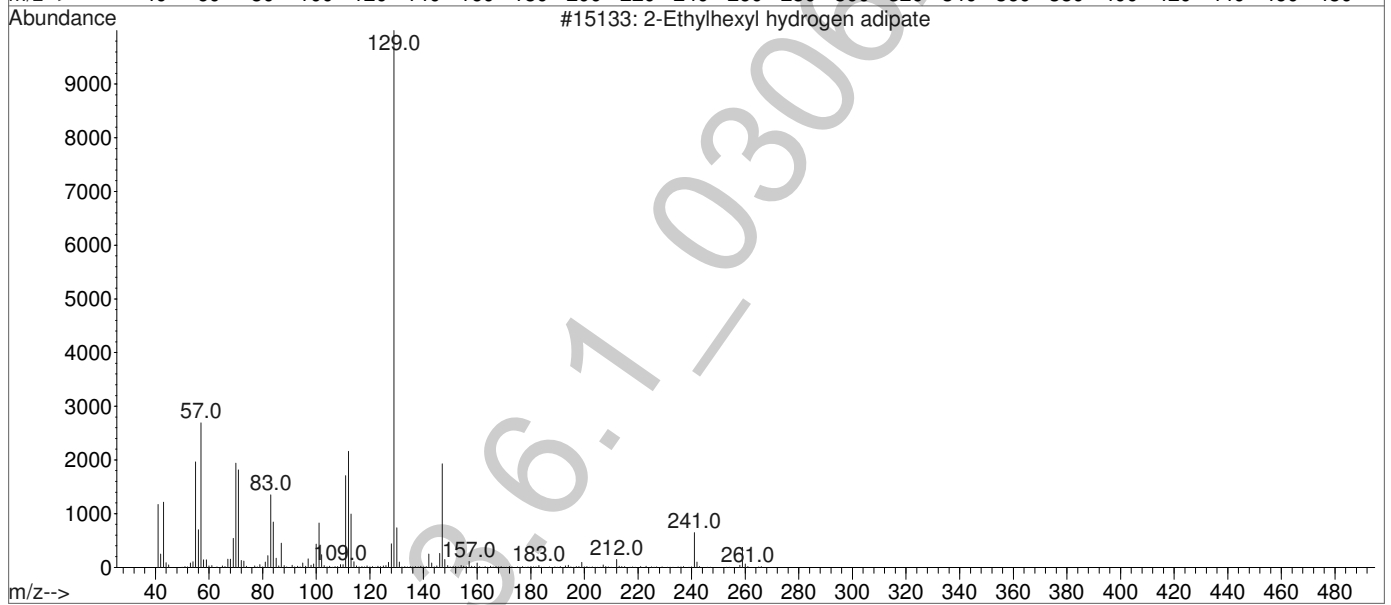
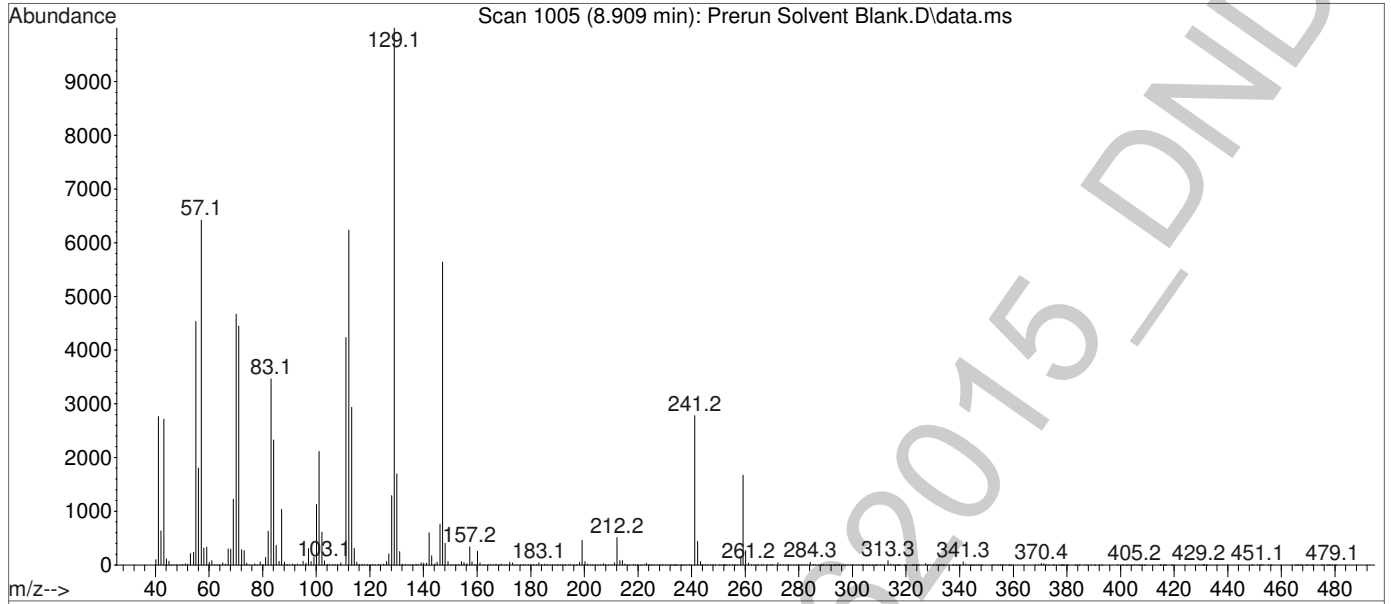


POC-AM-06.1-03009075-DND



File :C:\gcms\1\data\Blood\030615BN\Negative Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 06 Mar 2015 09:10 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0130
Misc Info : Analytical Method 3.6.1
Vial Number: 1

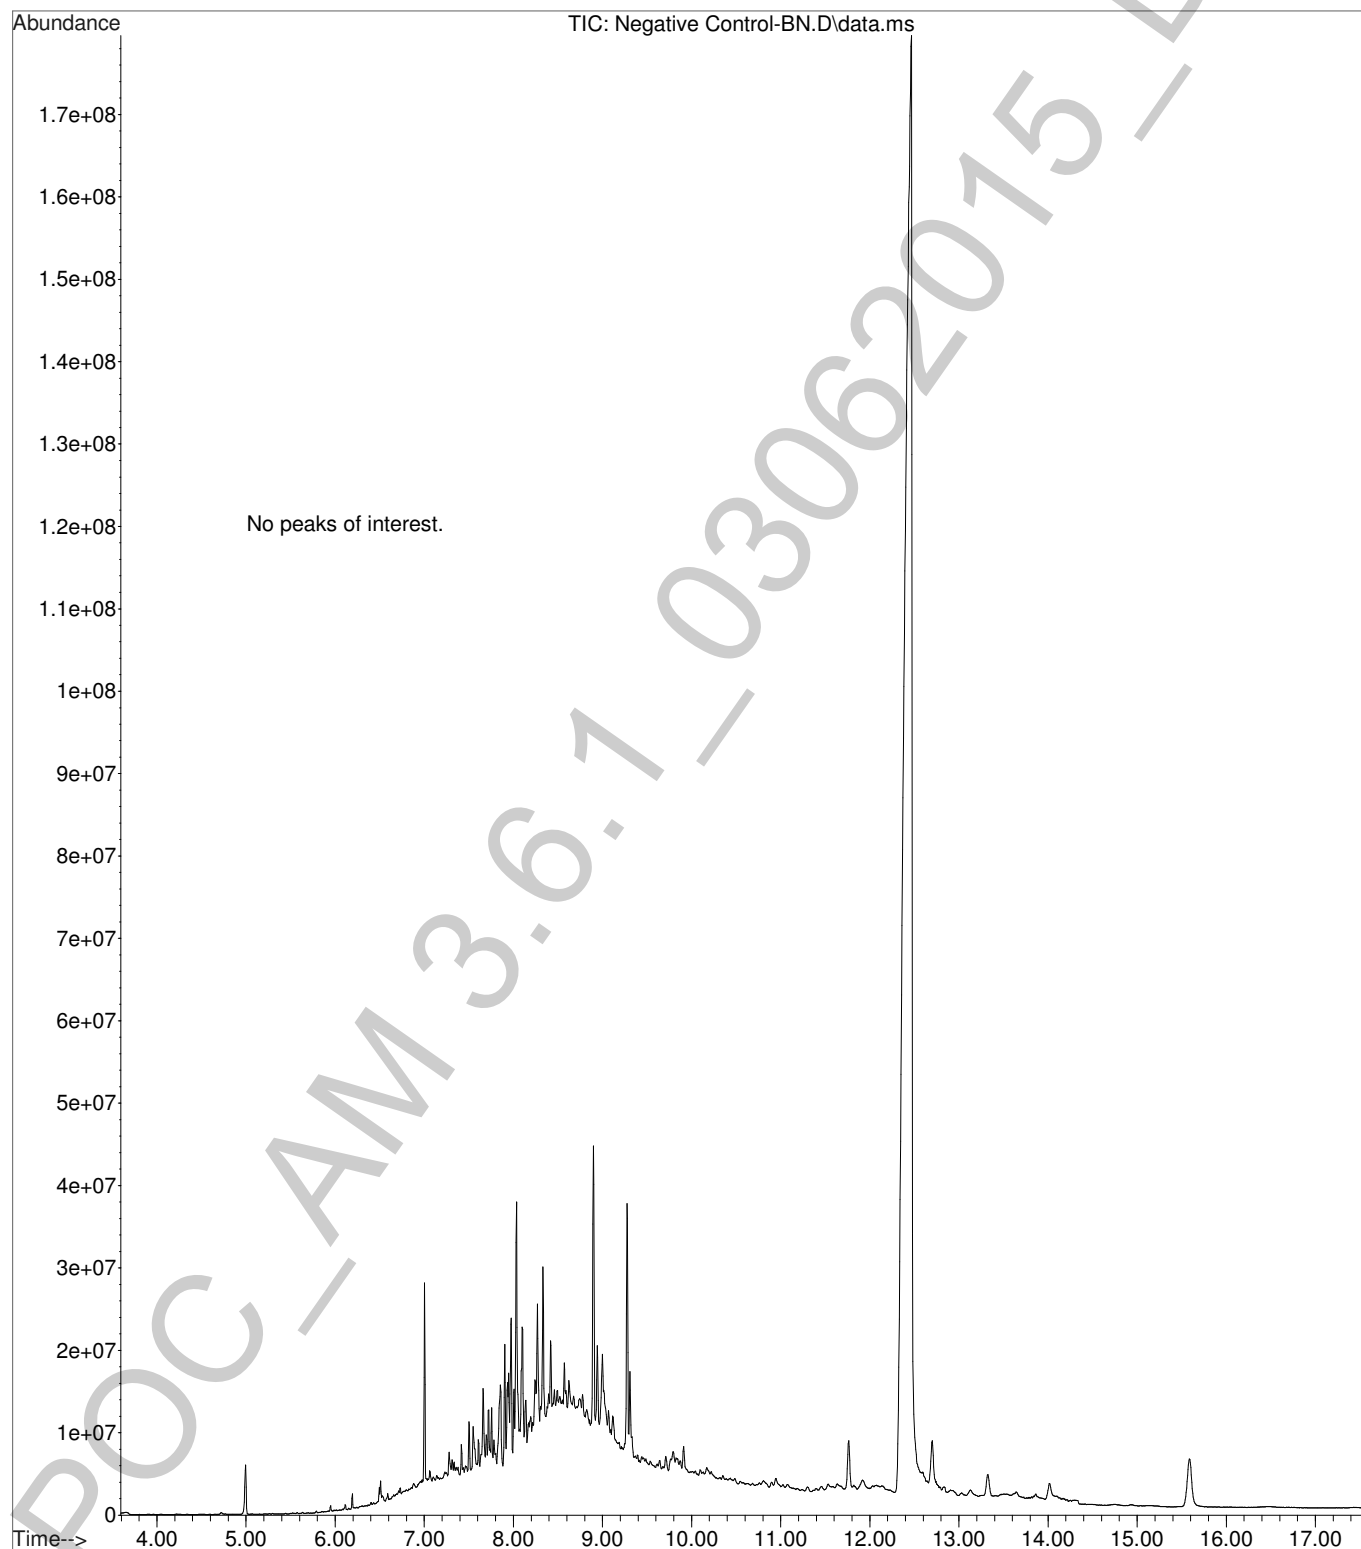


File :C:\gcms\1\data\Blood\030615BN\Negative Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 06 Mar 2015 09:10 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0130
Misc Info : Analytical Method 3.6.1
Vial Number: 1

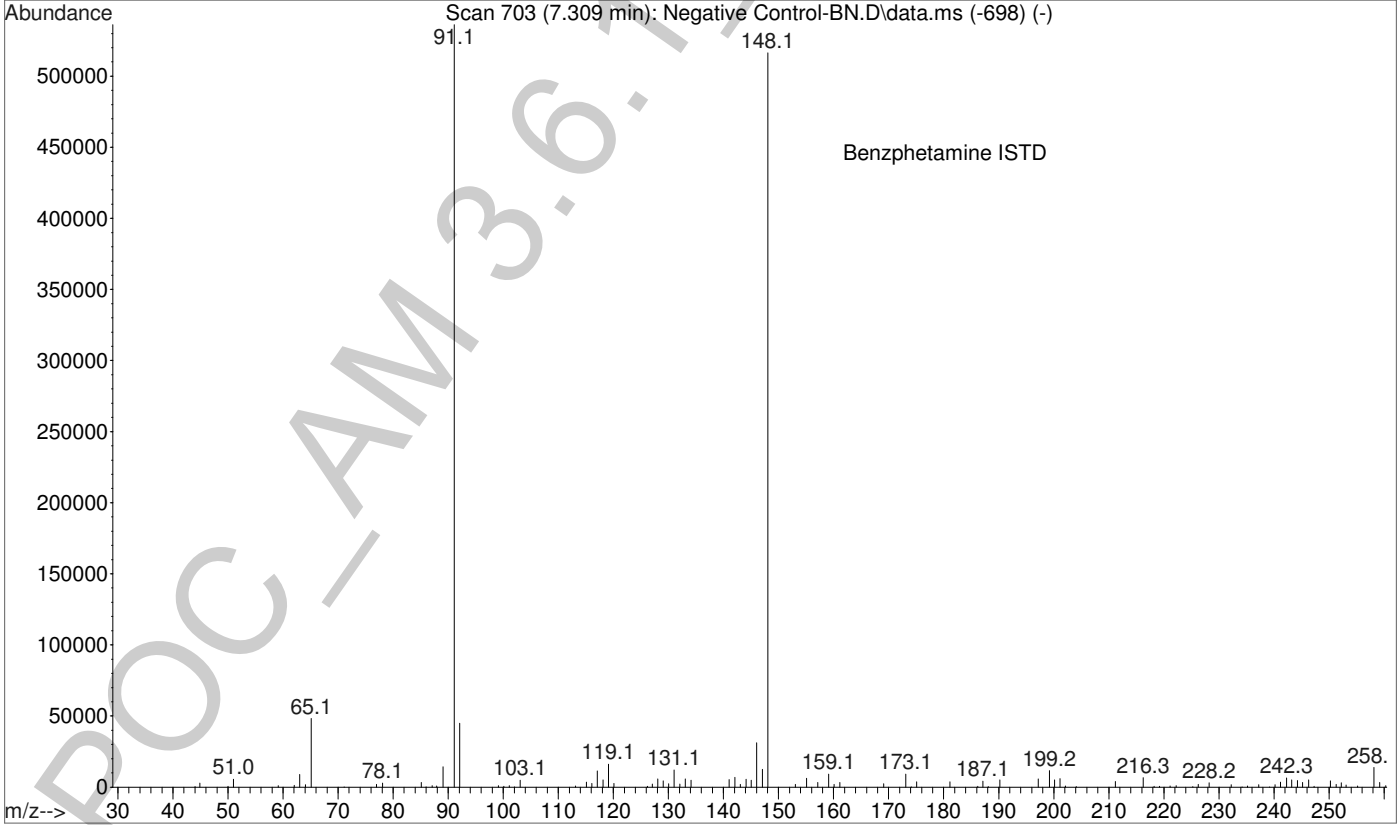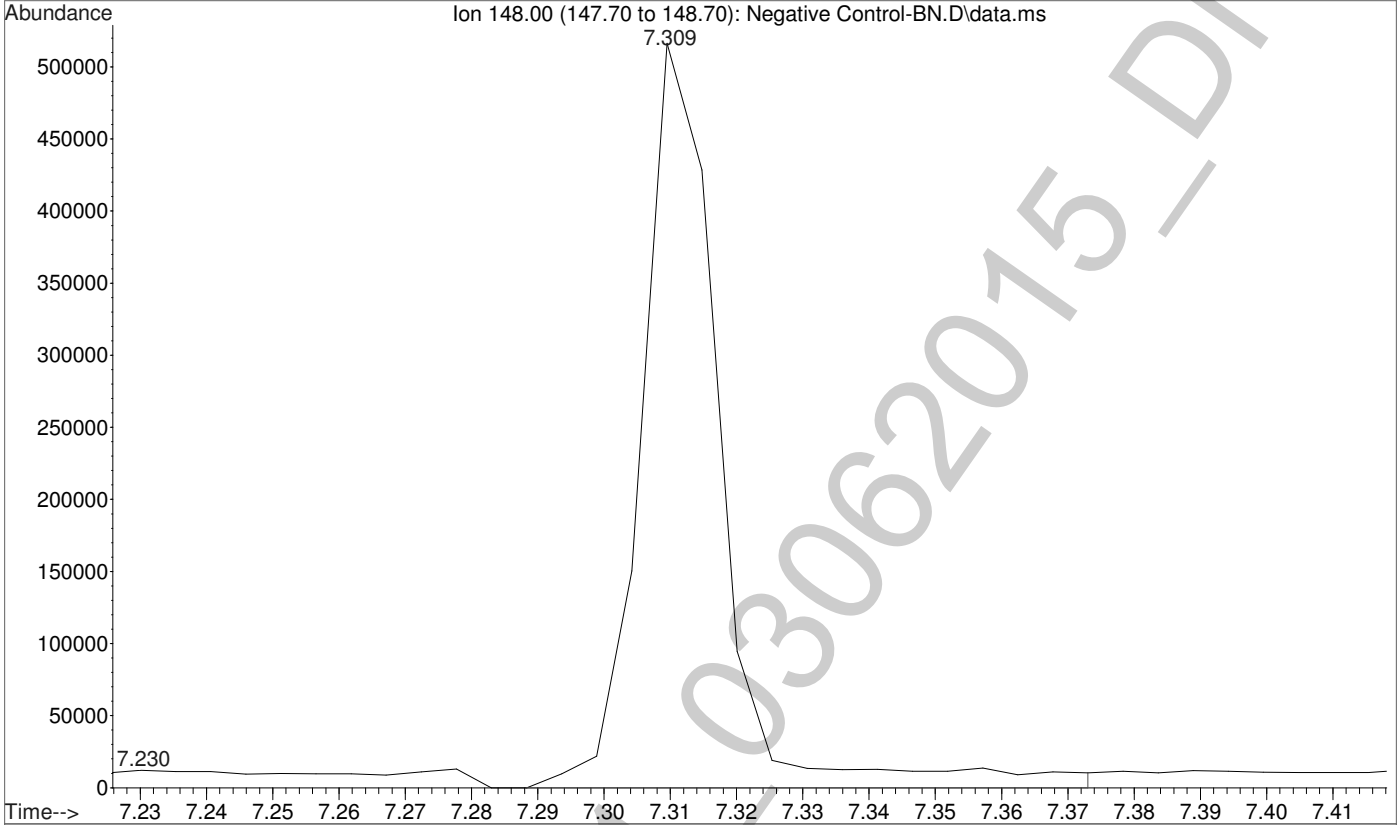



File :C:\gcms\1\data\Blood\030615BN\Negative Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 06 Mar 2015 09:10 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0130
Misc Info : Analytical Method 3.6.1
Vial Number: 1

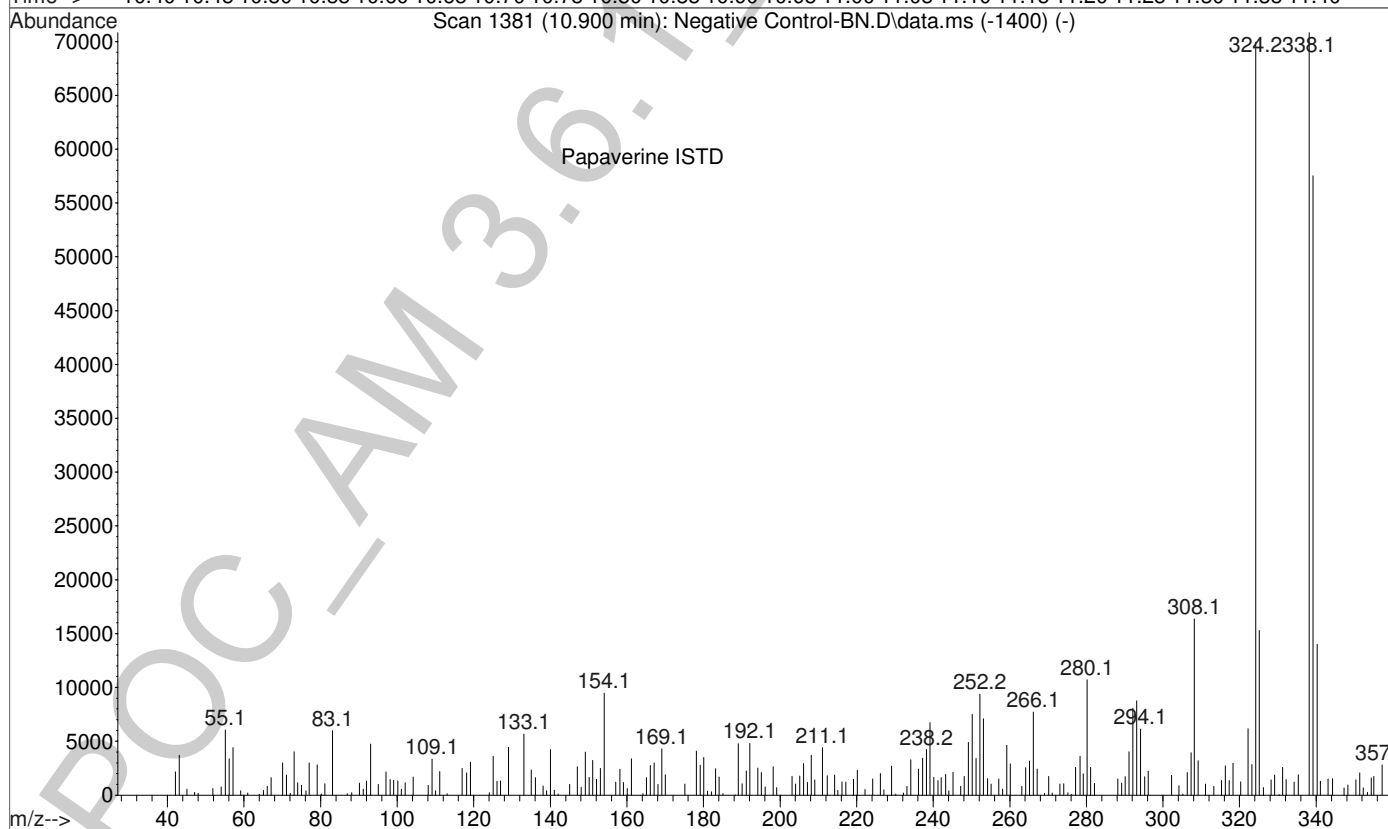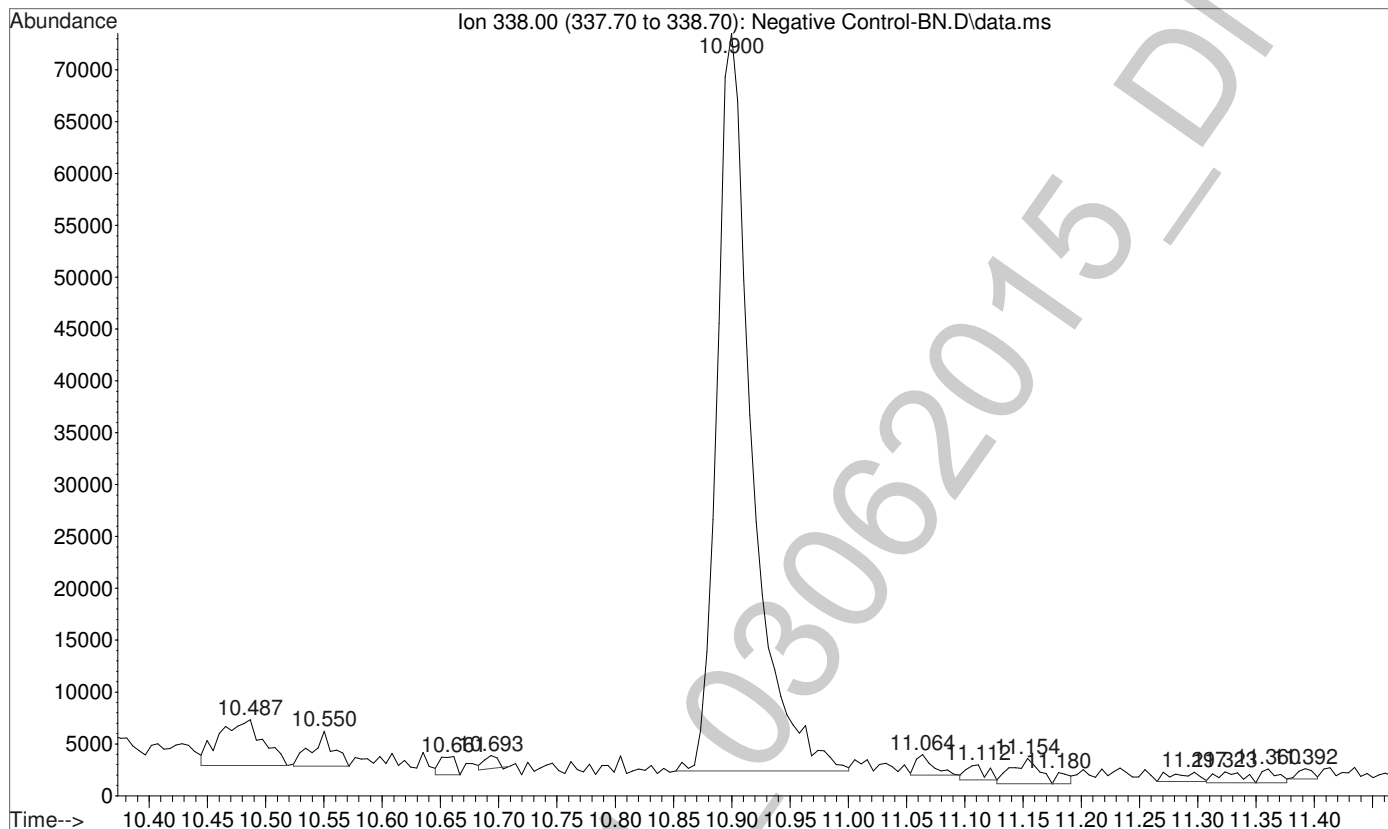



File :C:\gcms\1\data\Blood\030615BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 06 Mar 2015 09:33 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

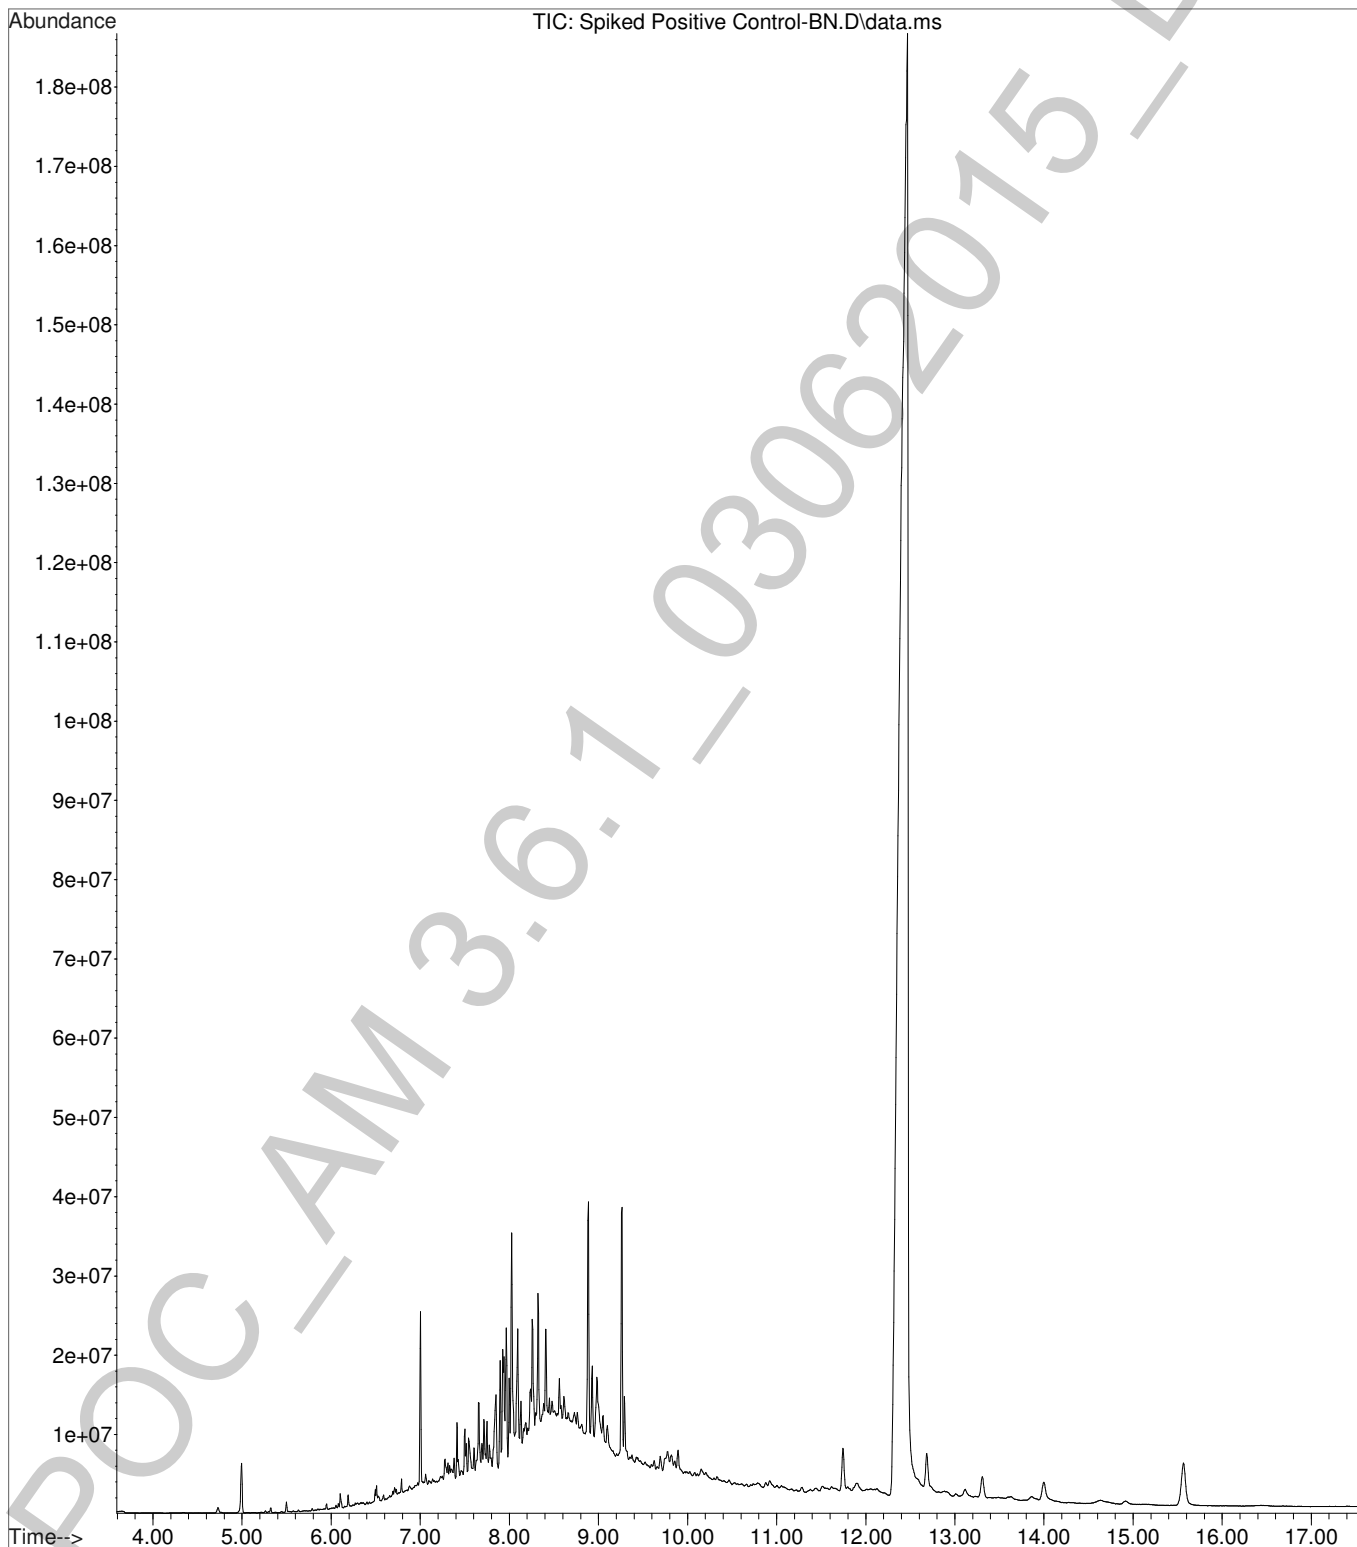



File :C:\gcms\1\data\Blood\030615BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 06 Mar 2015 09:33 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

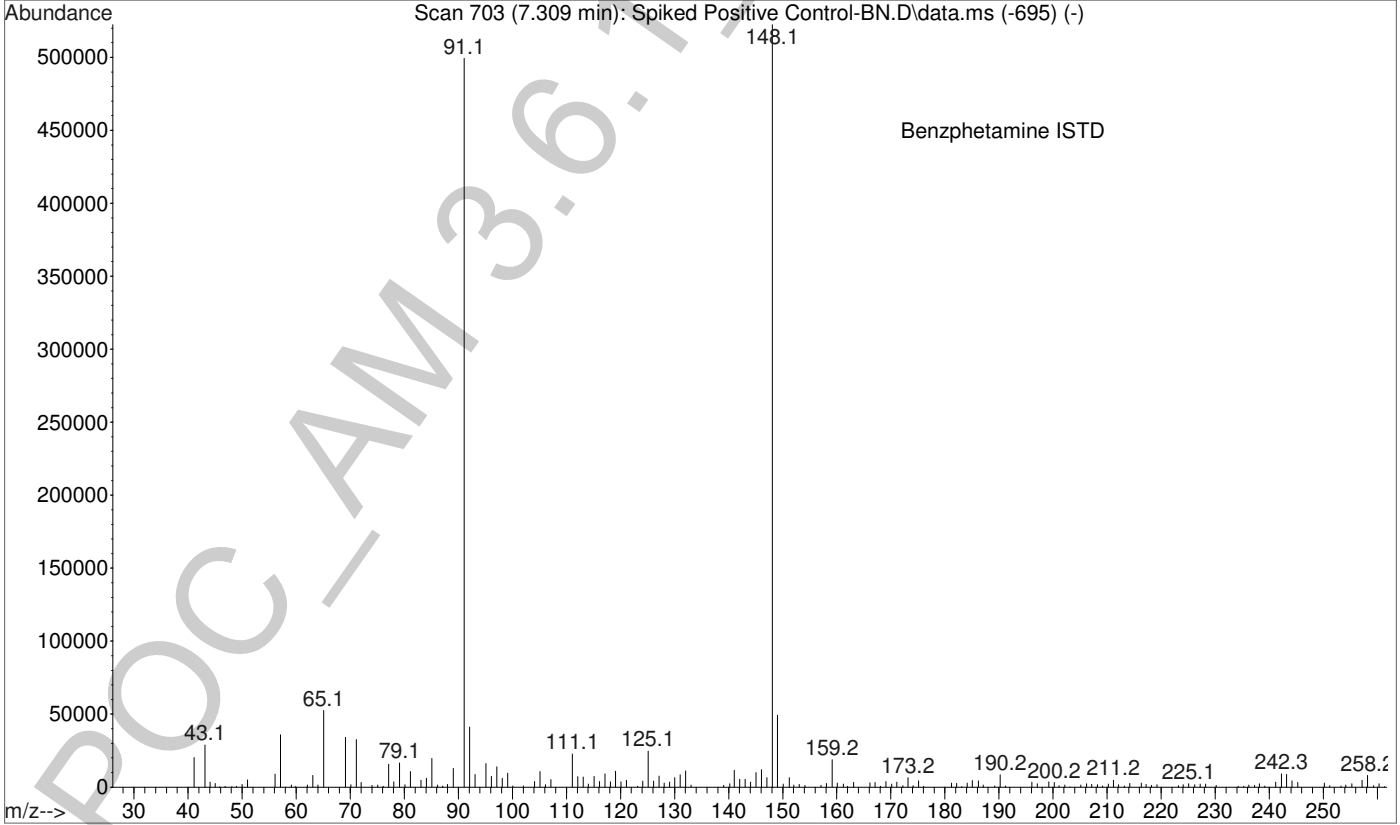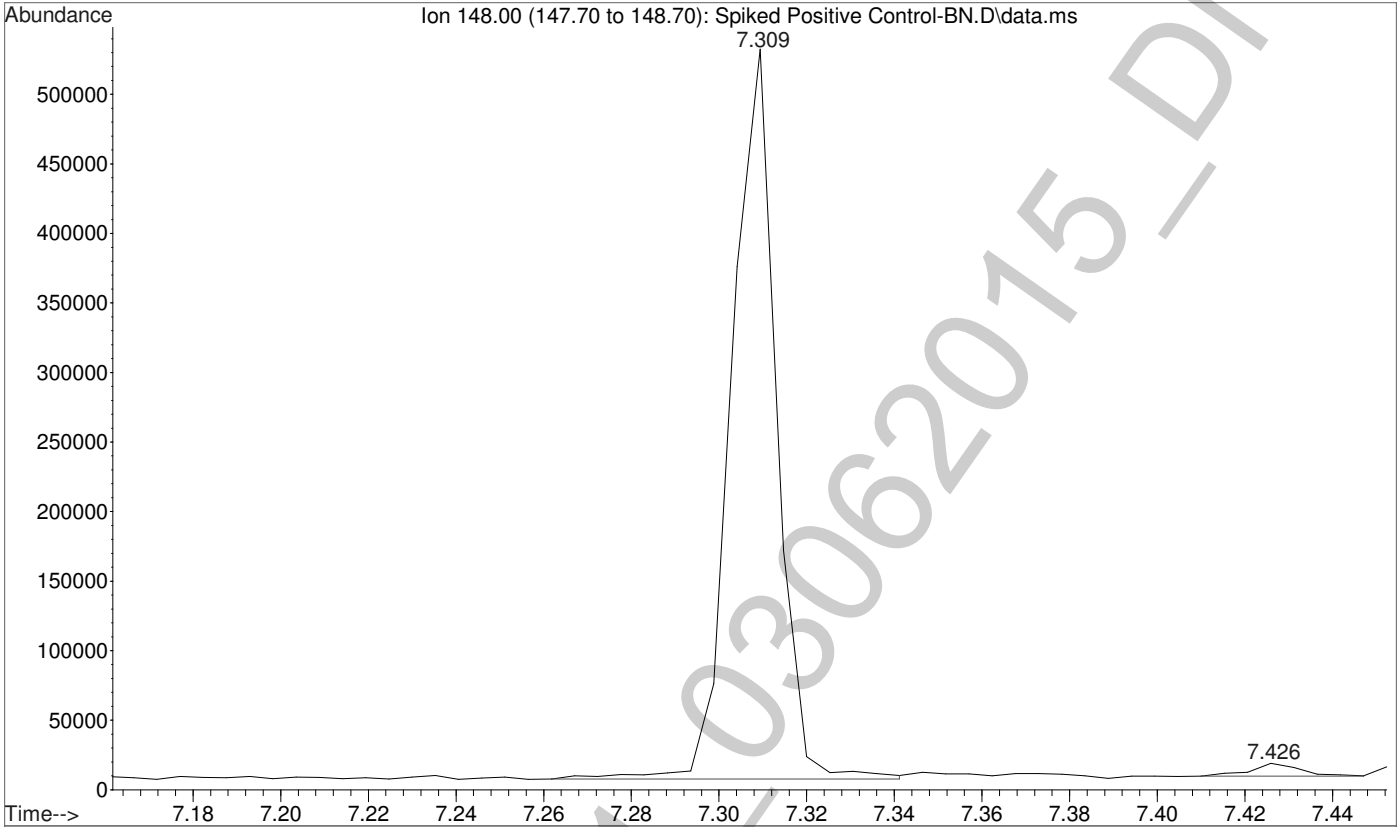



File :C:\gcms\1\data\Blood\030615BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 06 Mar 2015 09:33 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

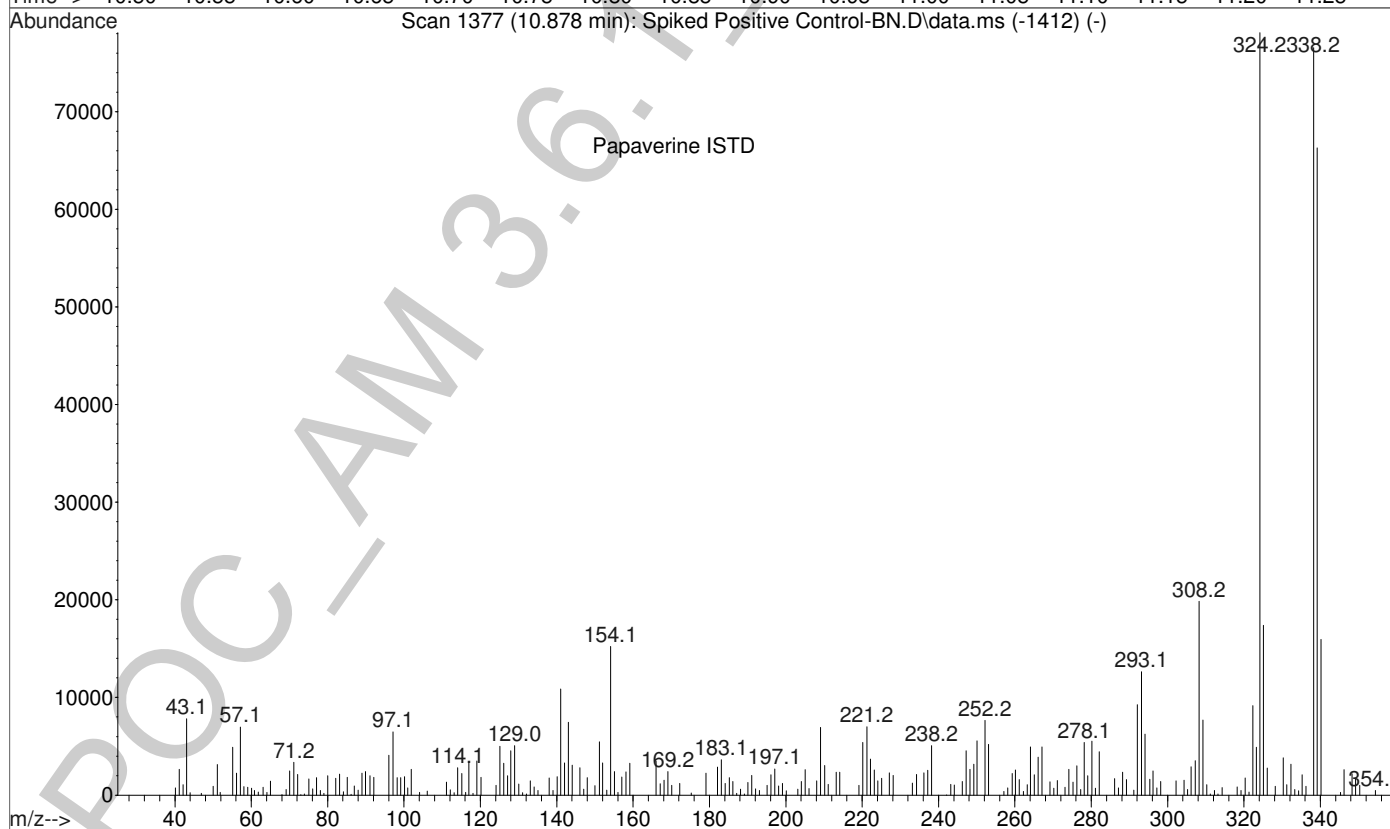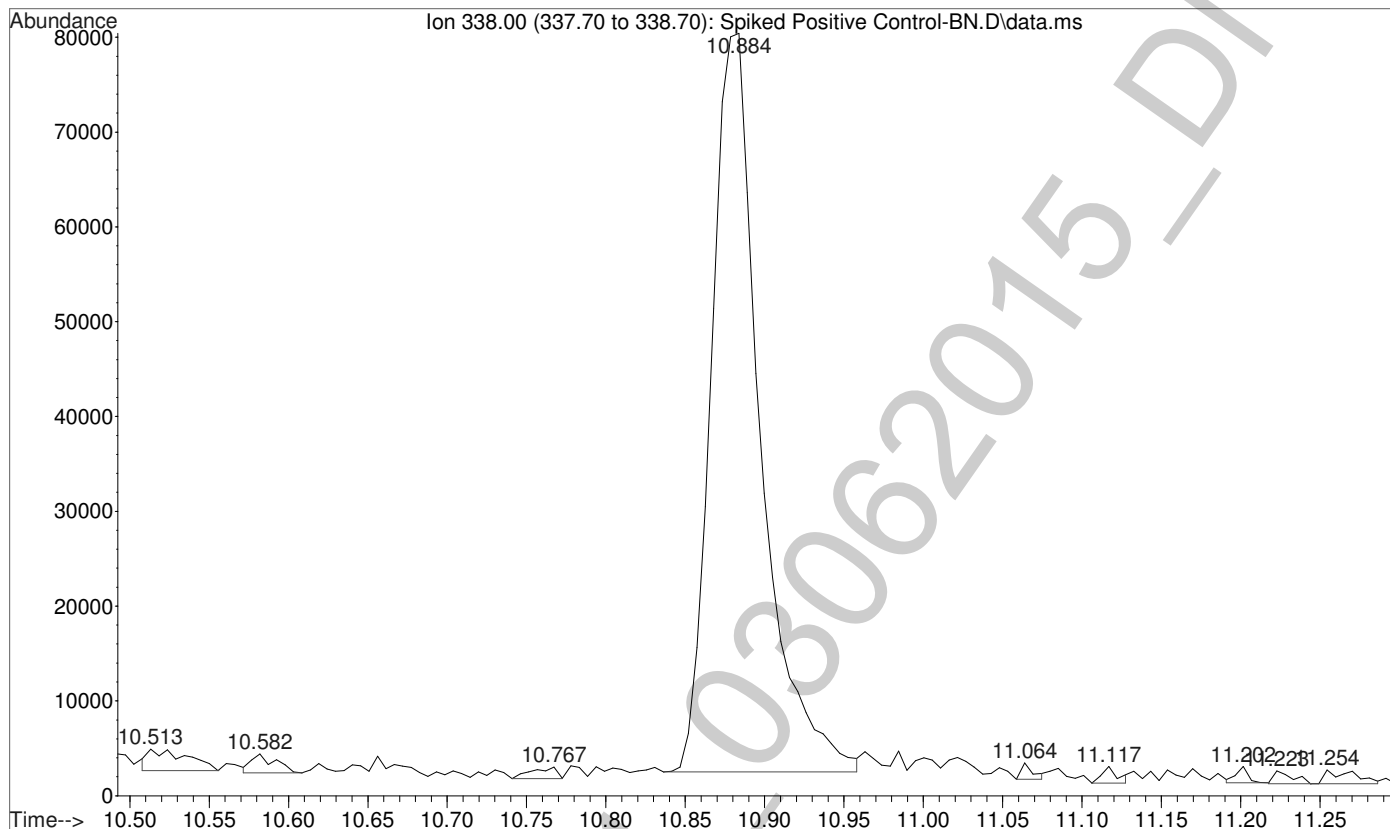



File :C:\gcms\1\data\Blood\030615BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 06 Mar 2015 09:33 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

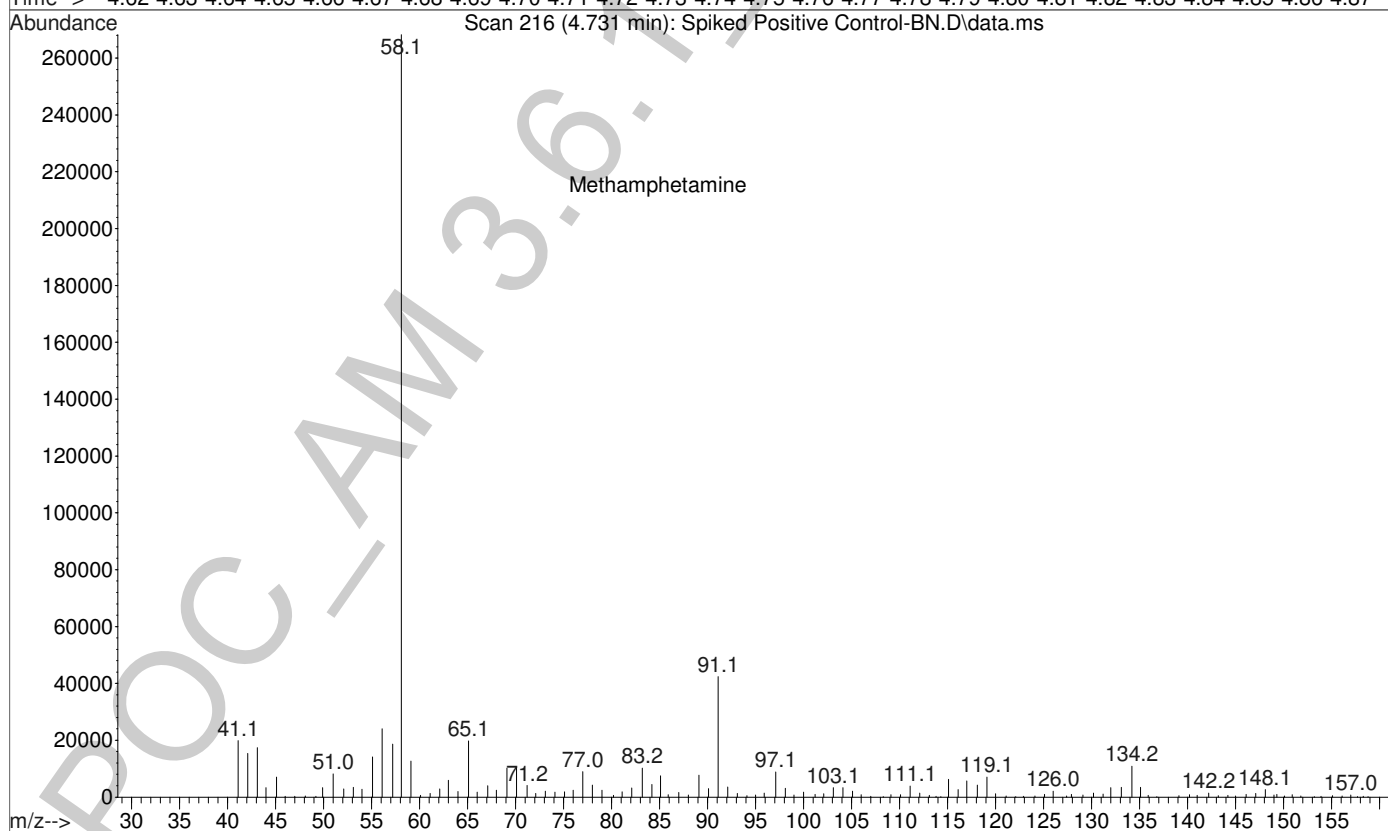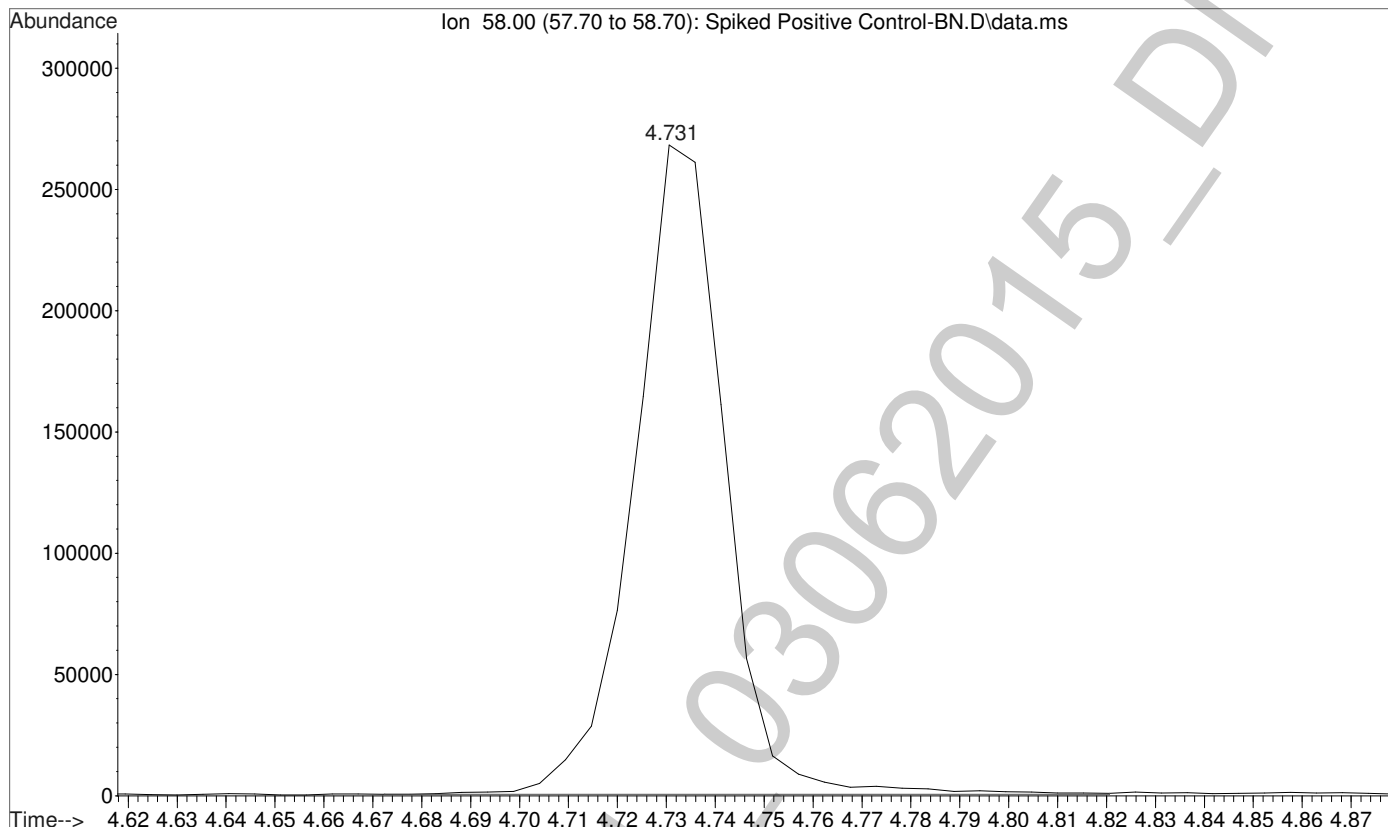



File :C:\gcms\1\data\Blood\030615BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 06 Mar 2015 09:33 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

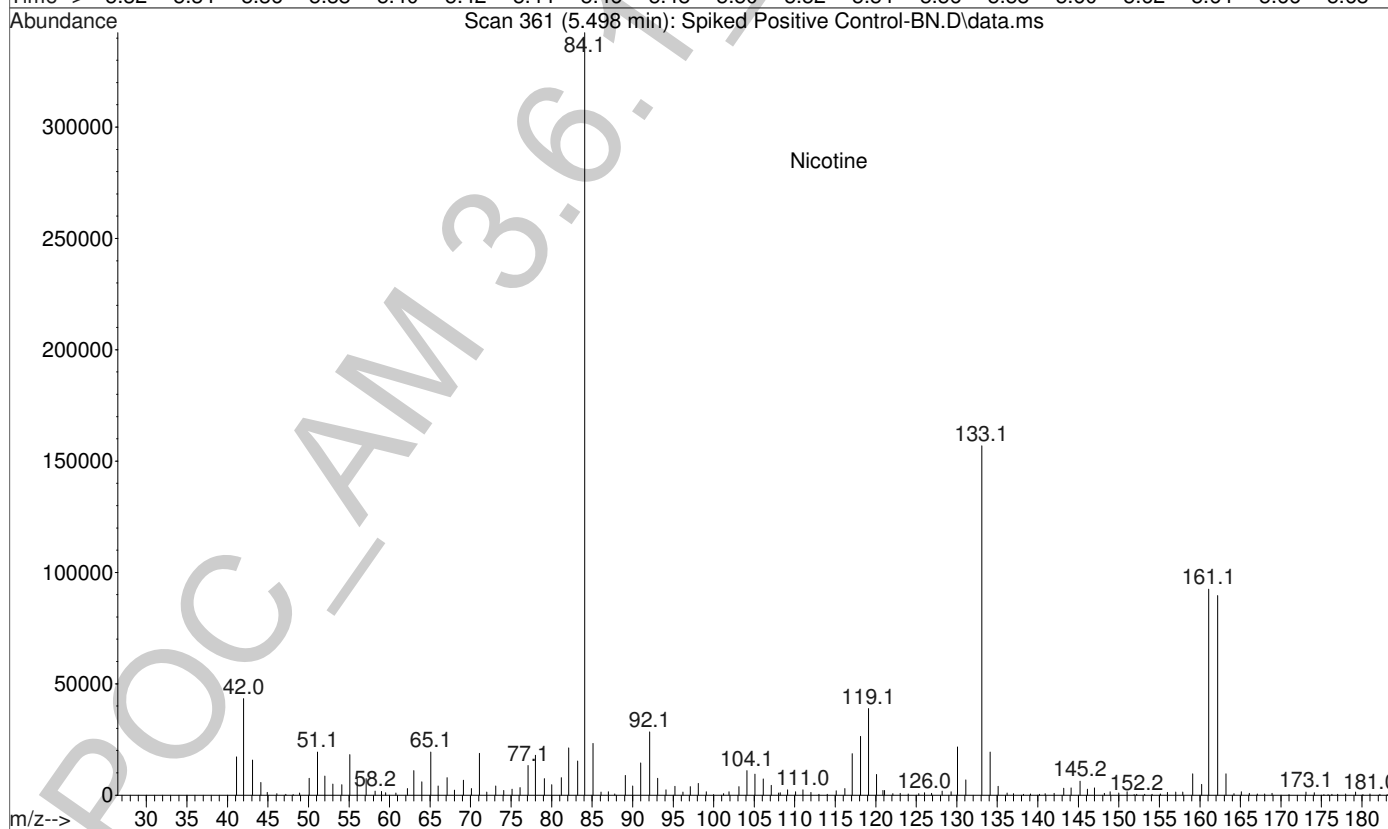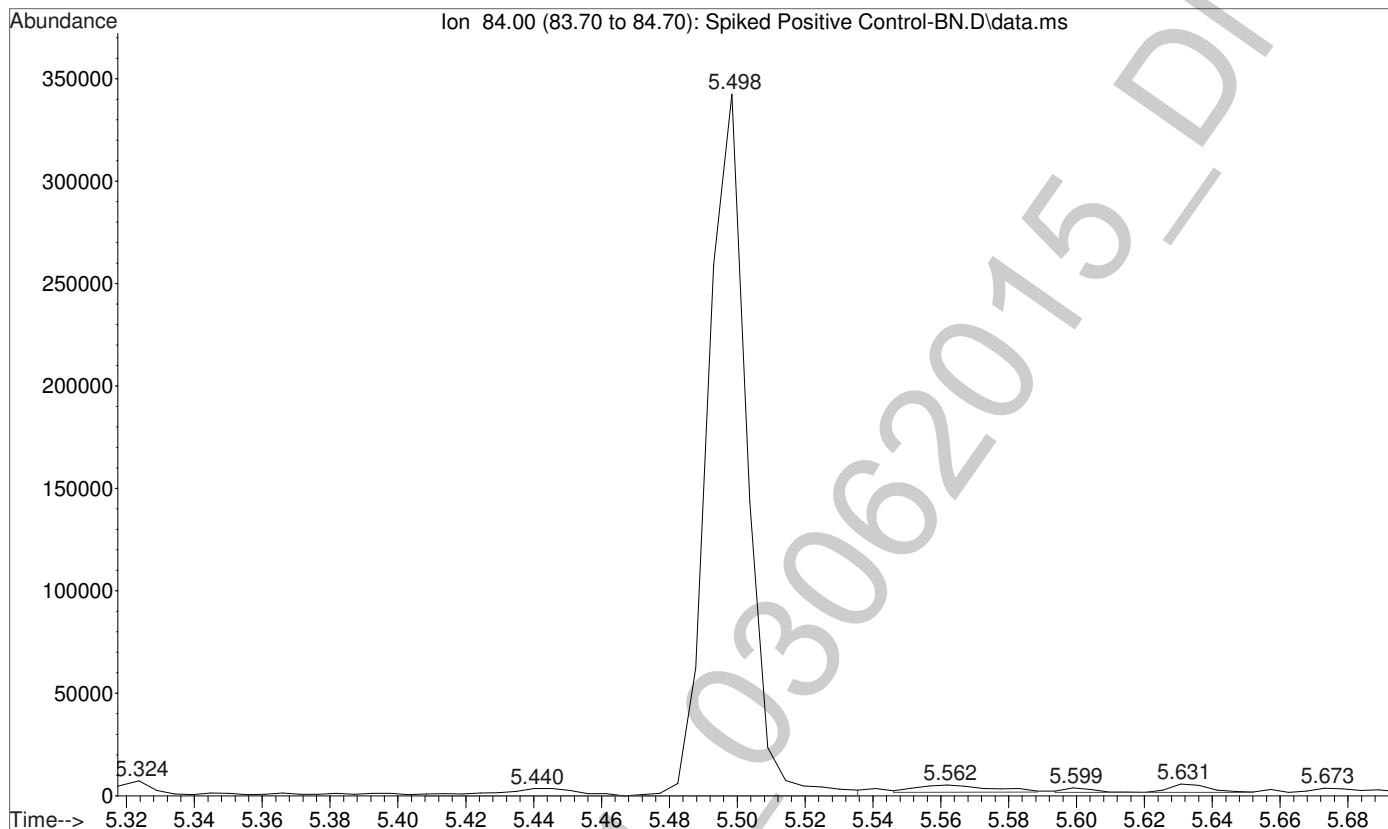



File :C:\gcms\1\data\Blood\030615BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 06 Mar 2015 09:33 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

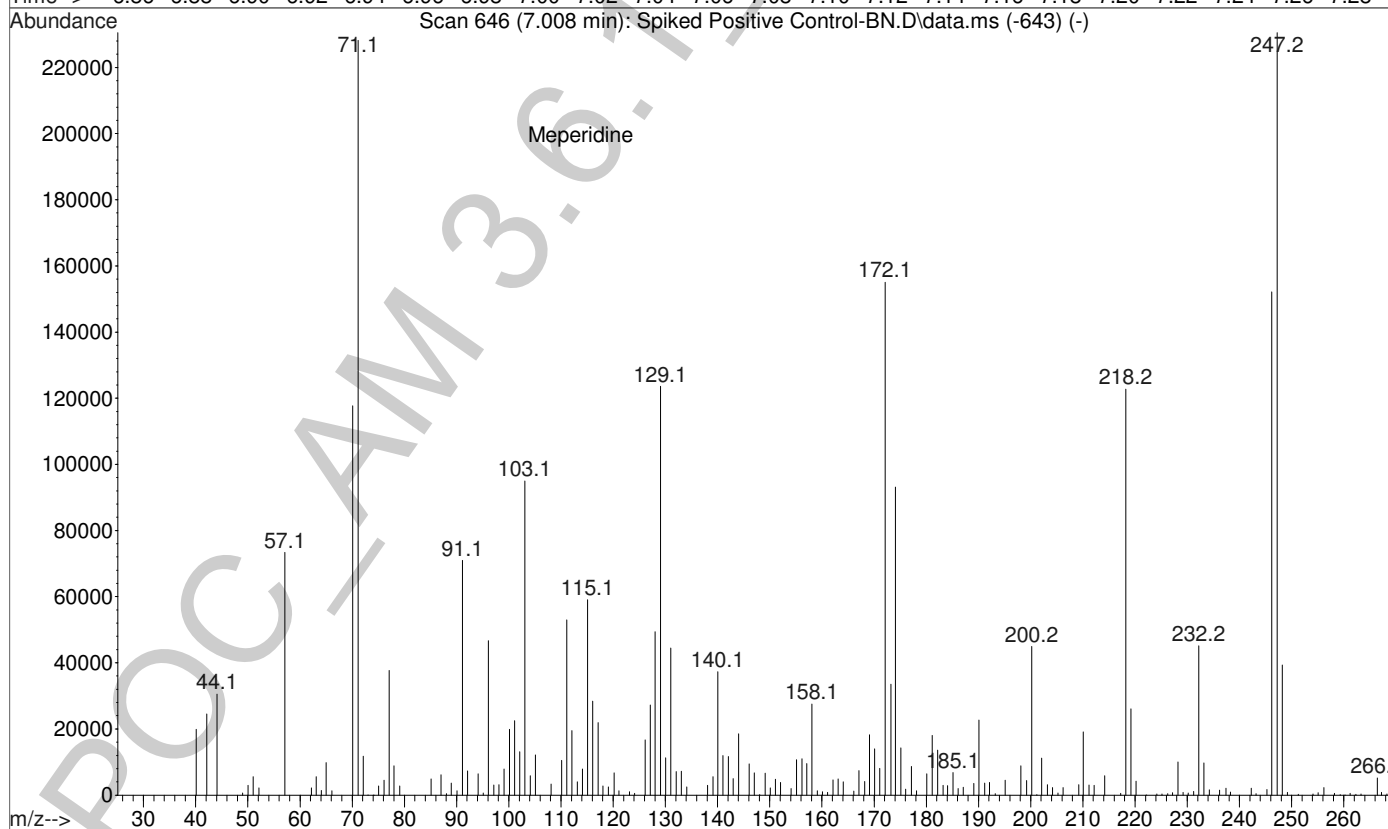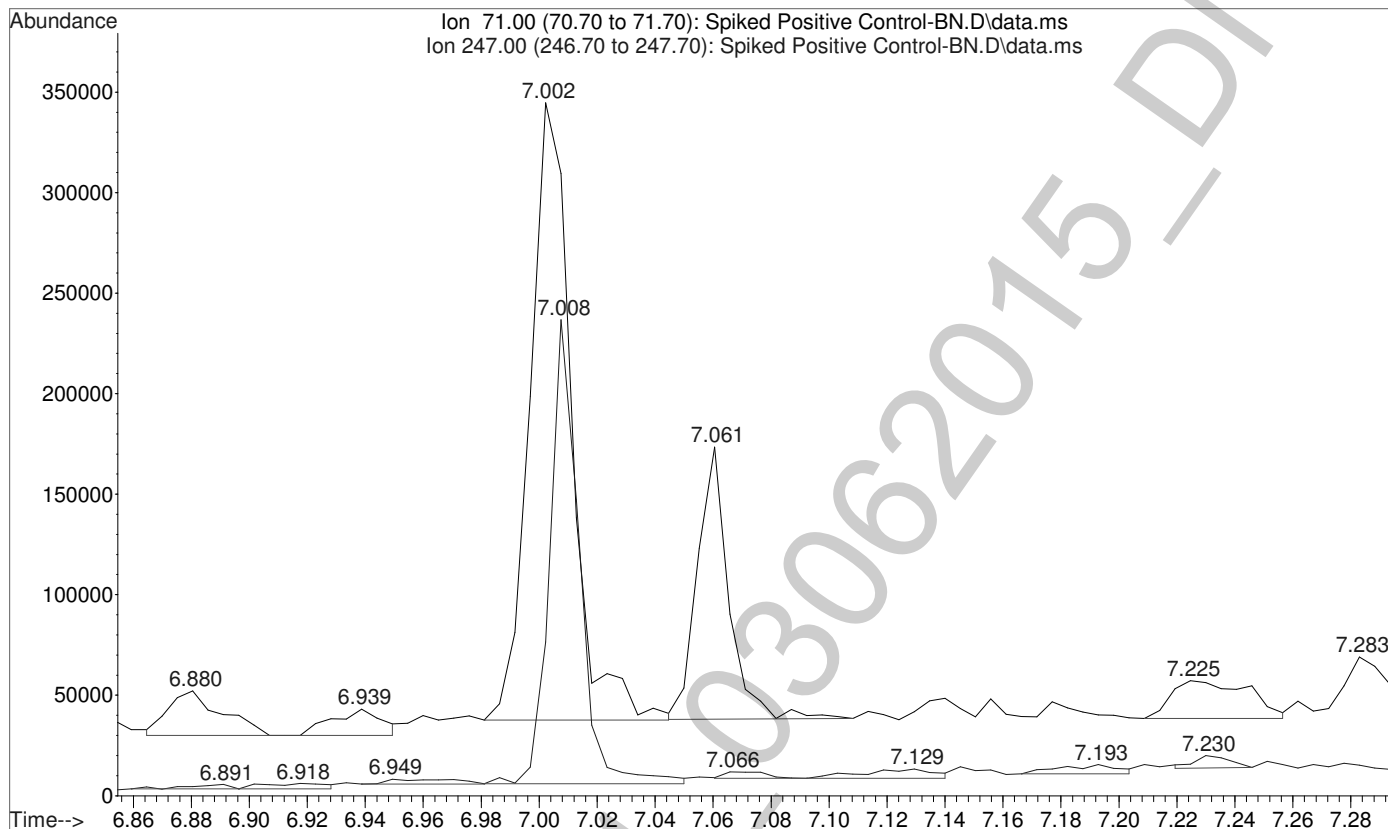



File :C:\gcms\1\data\Blood\030615BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 06 Mar 2015 09:33 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

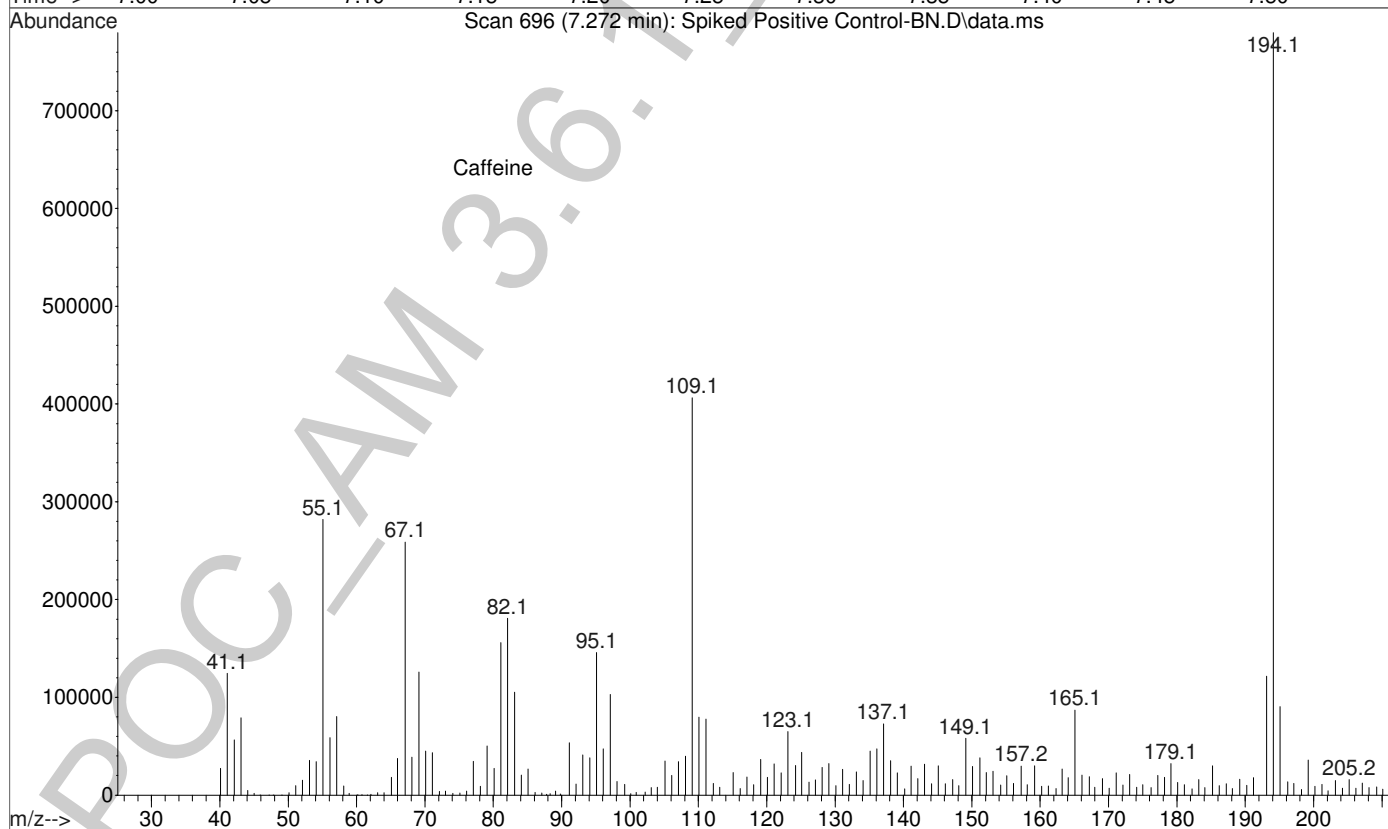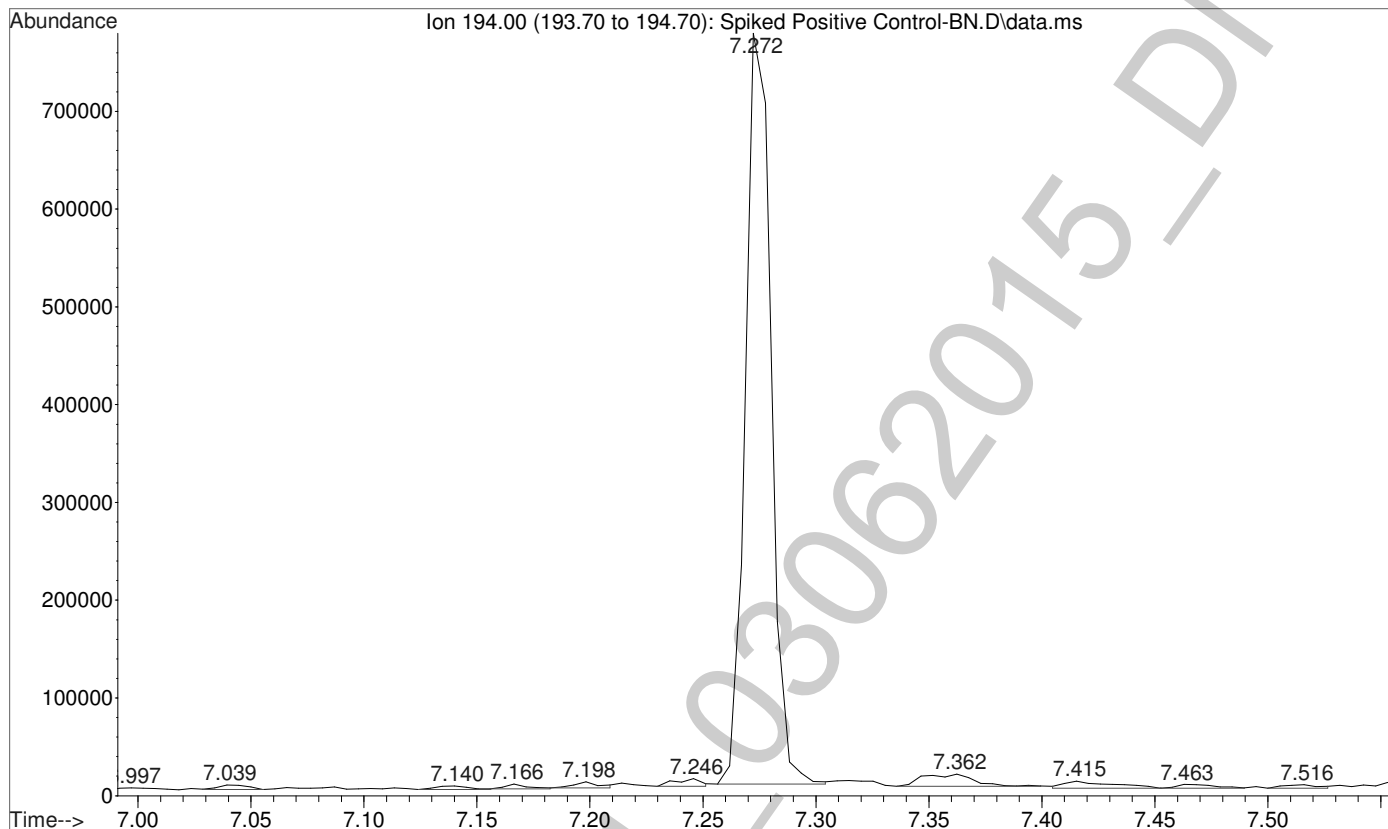



File :C:\gcms\1\data\Blood\030615BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 06 Mar 2015 09:33 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

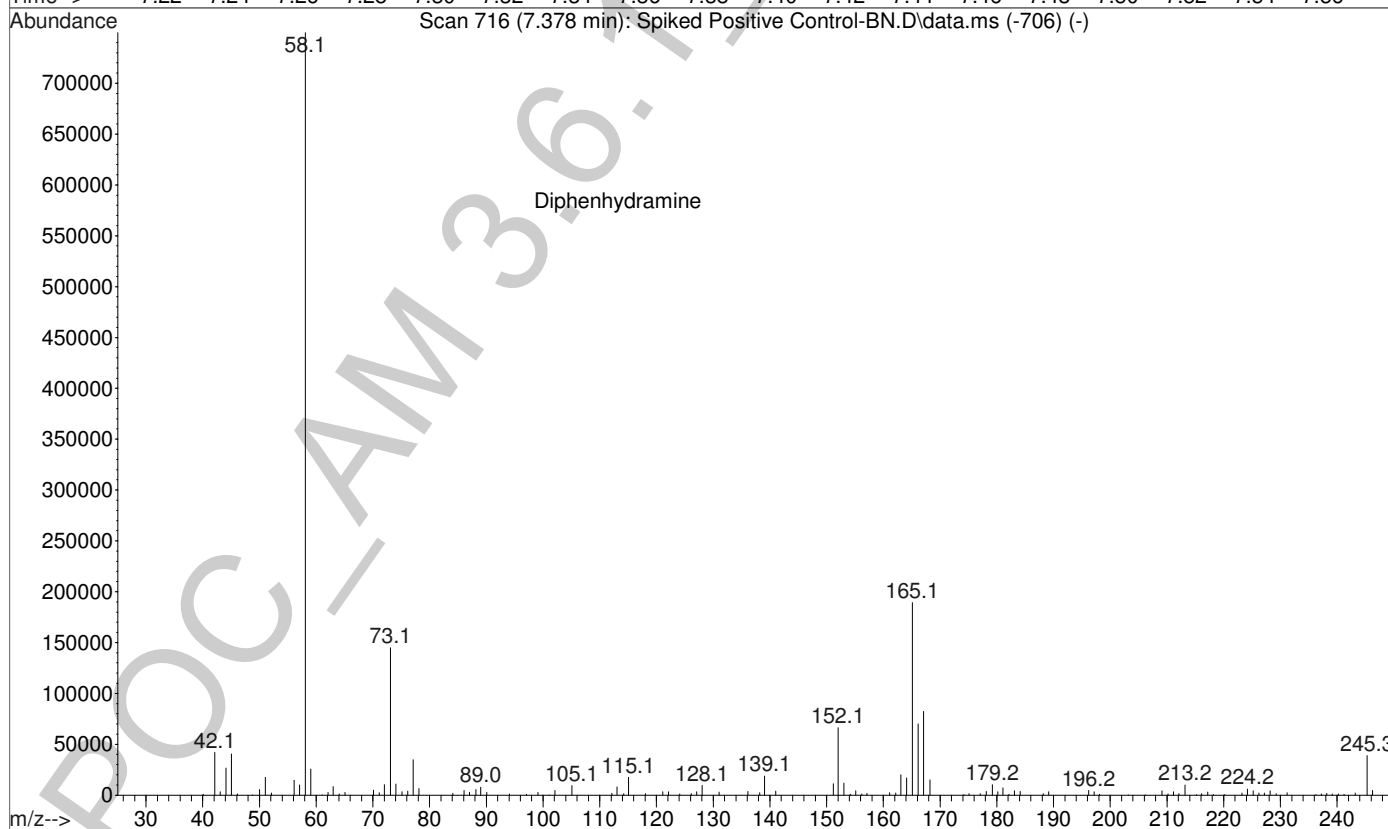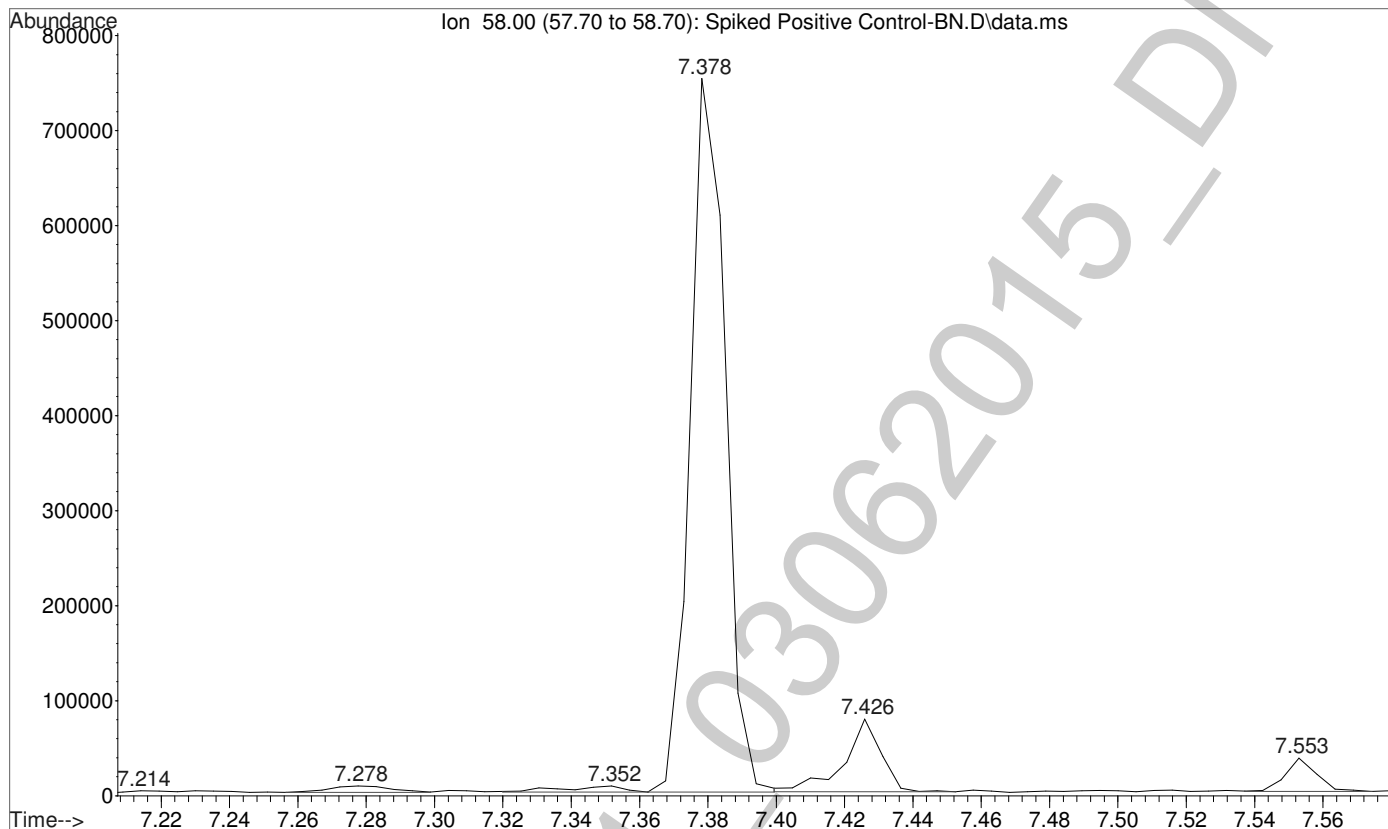



File :C:\gcms\1\data\Blood\030615BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 06 Mar 2015 09:33 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

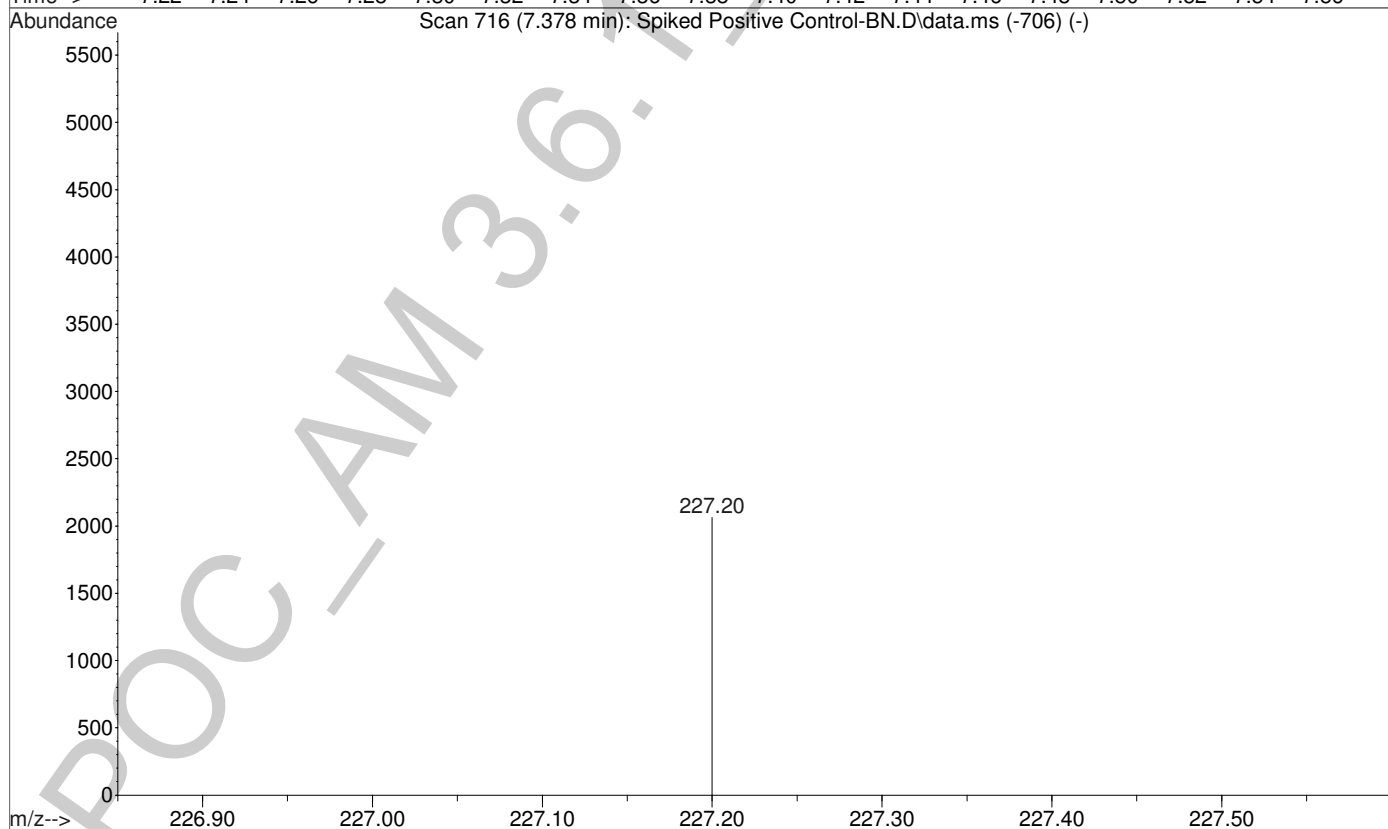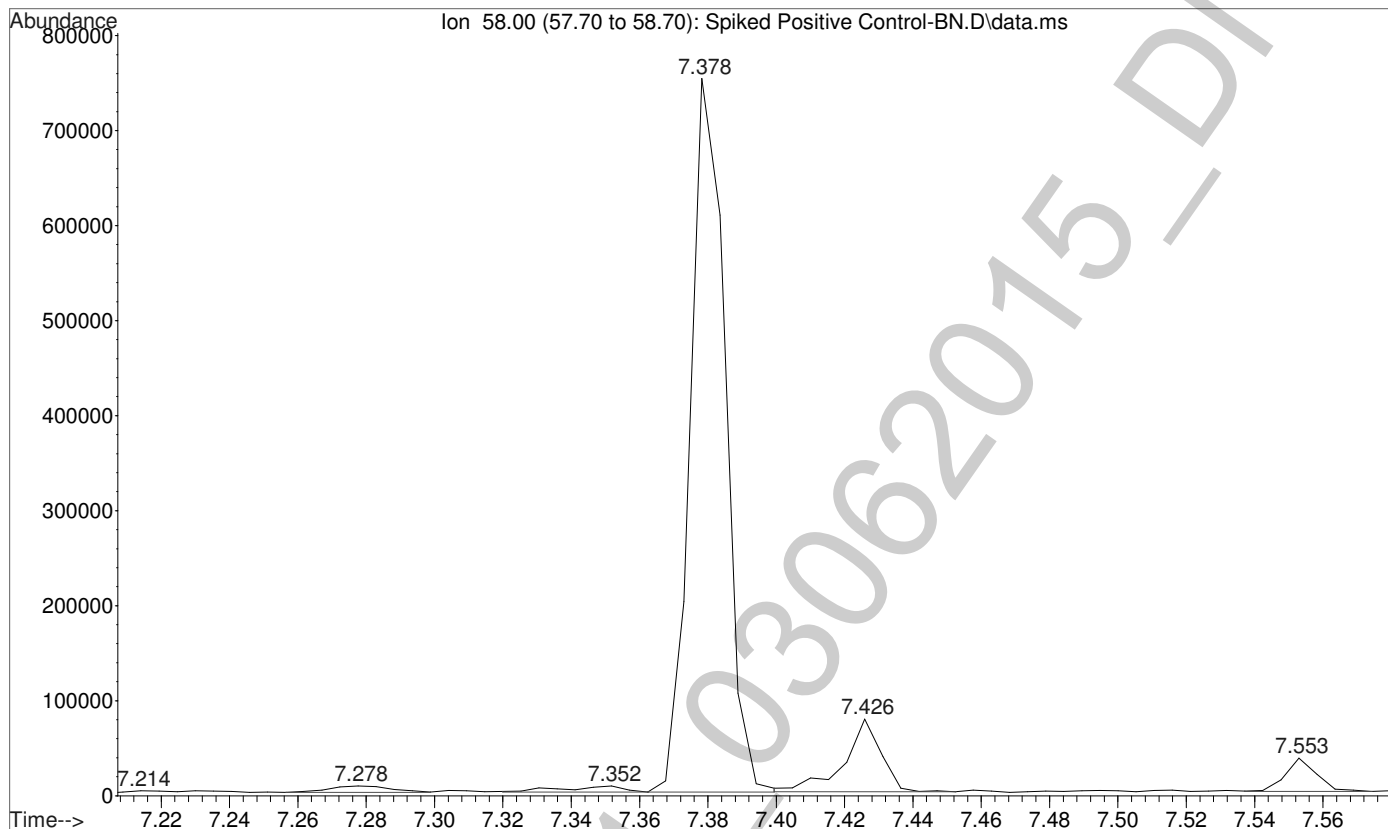



File :C:\gcms\1\data\Blood\030615BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 06 Mar 2015 09:33 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

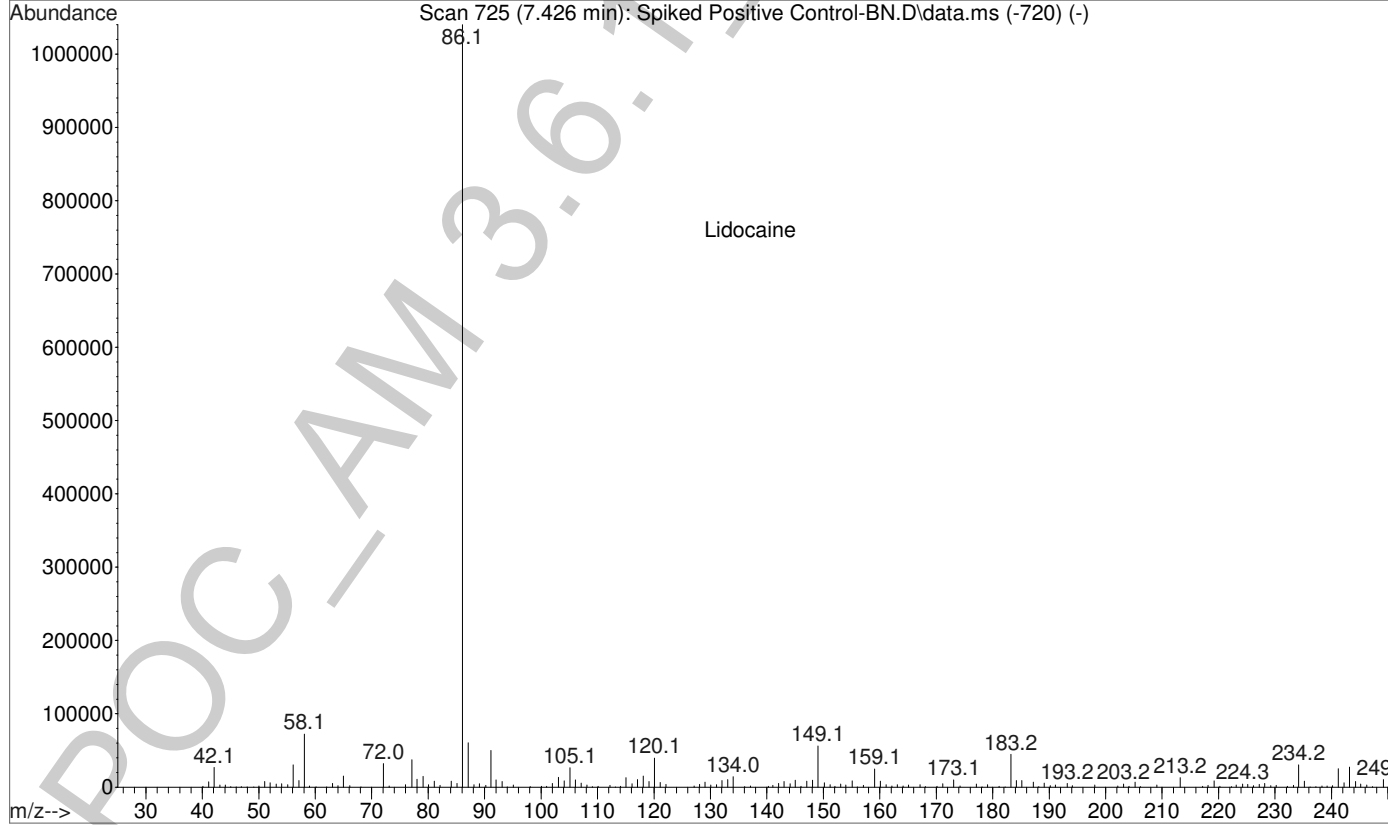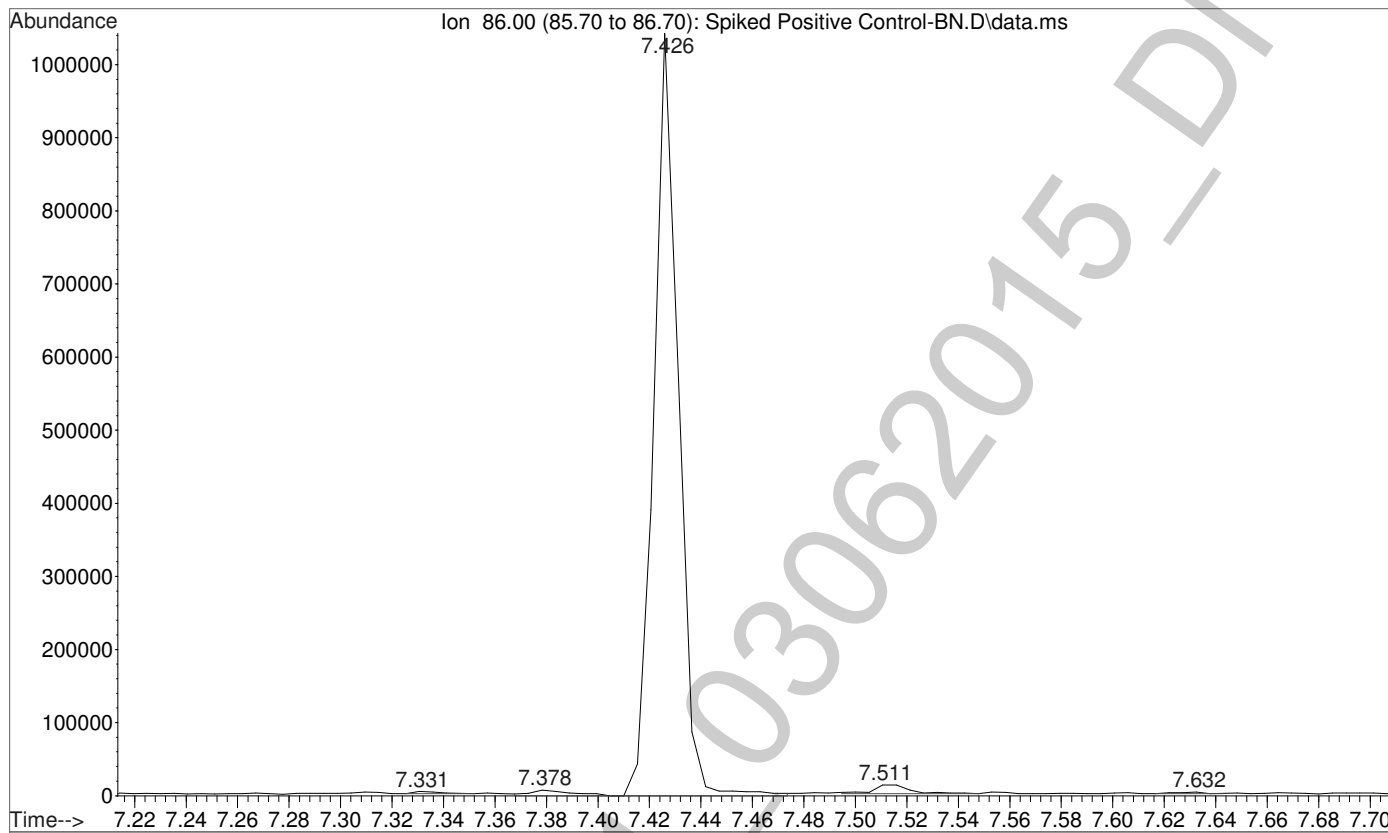



File :C:\gcms\1\data\Blood\030615BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 06 Mar 2015 09:33 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

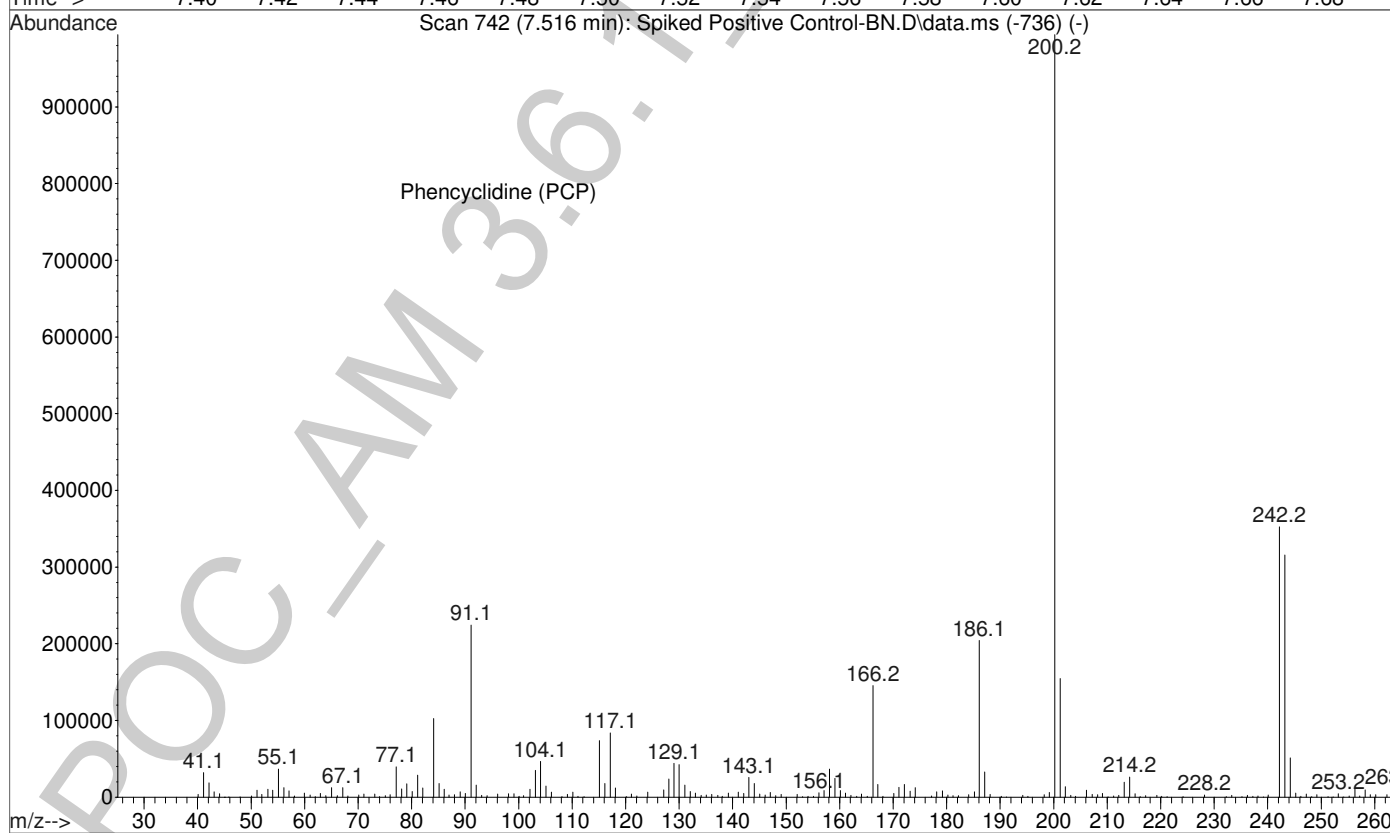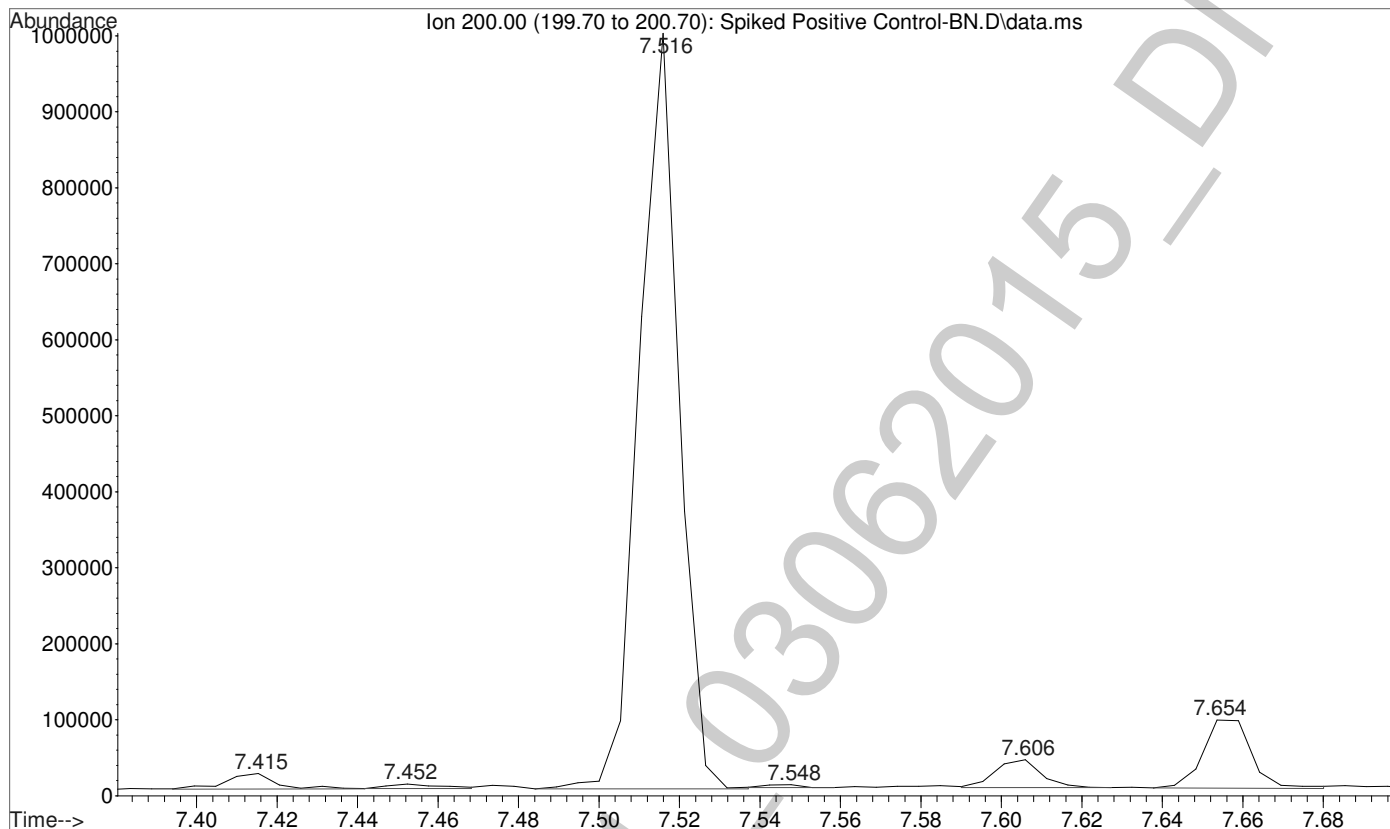



File :C:\gcms\1\data\Blood\030615BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 06 Mar 2015 09:33 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

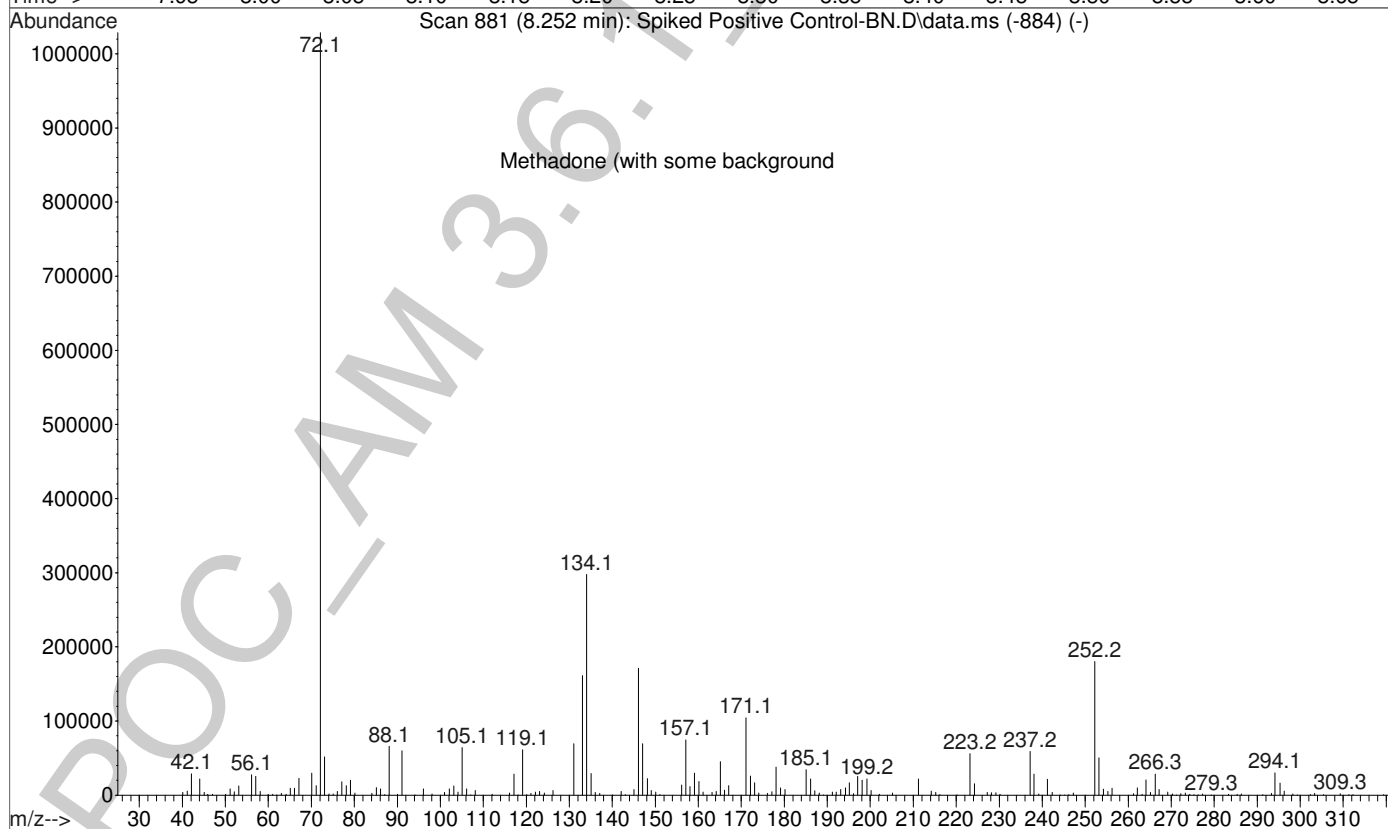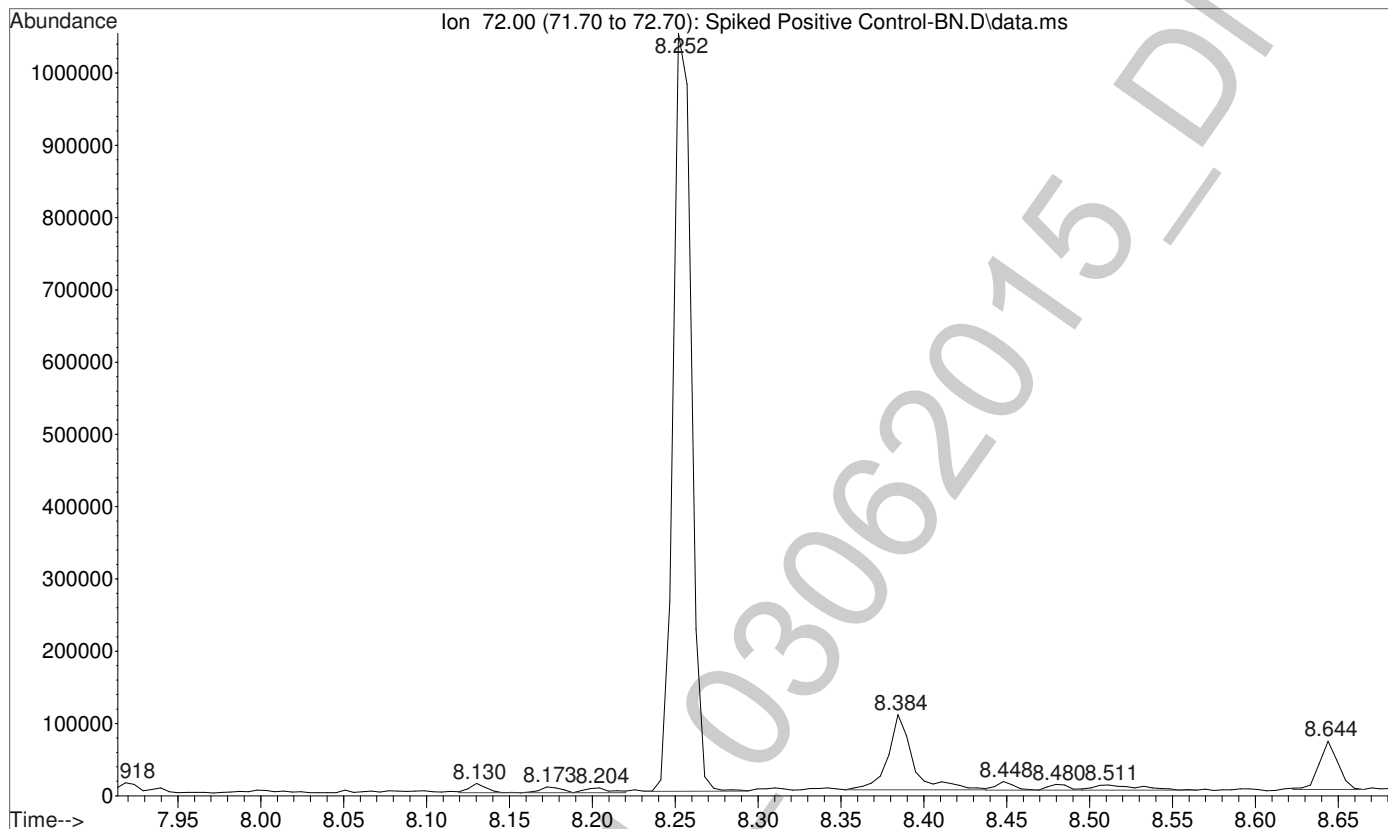



File :C:\gcms\1\data\Blood\030615BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 06 Mar 2015 09:33 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

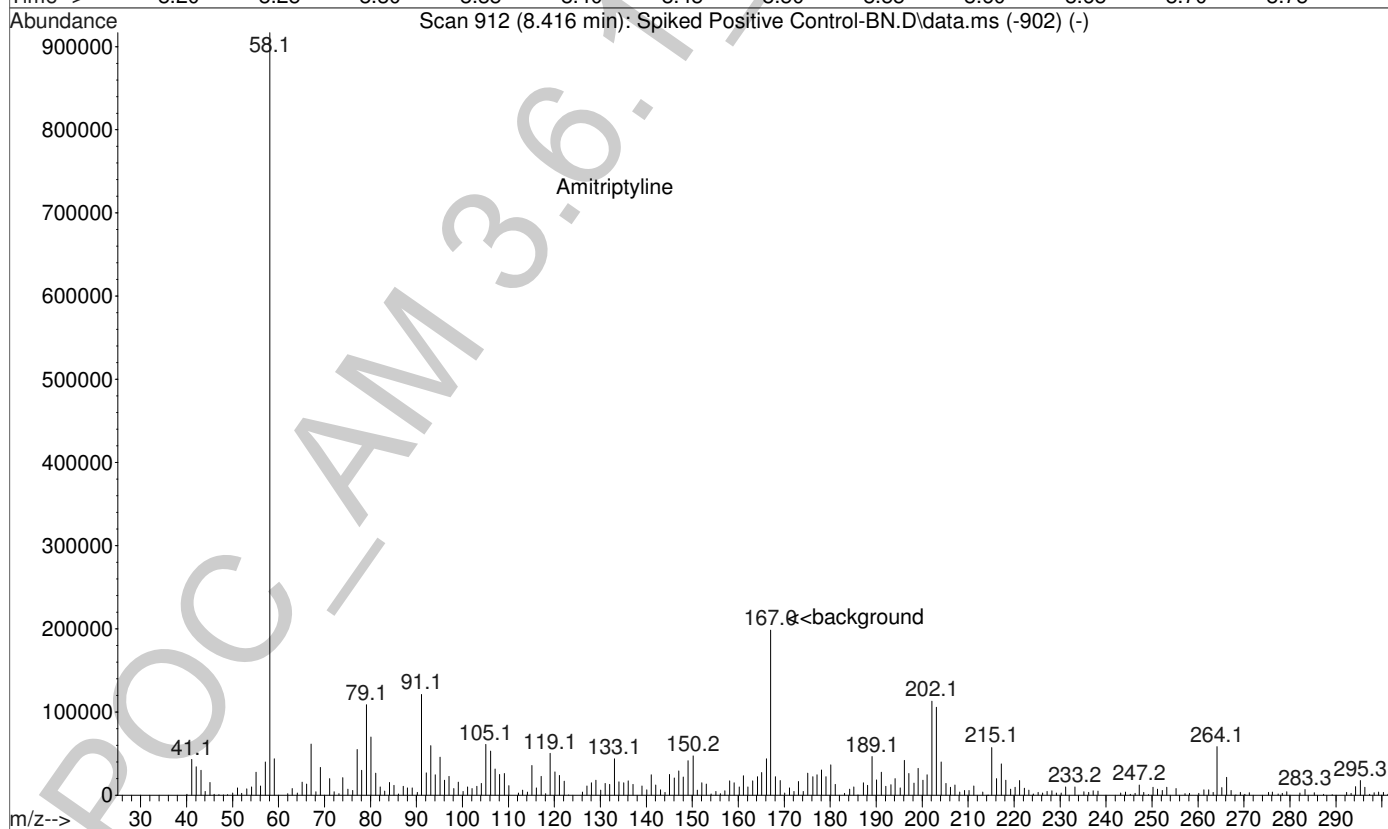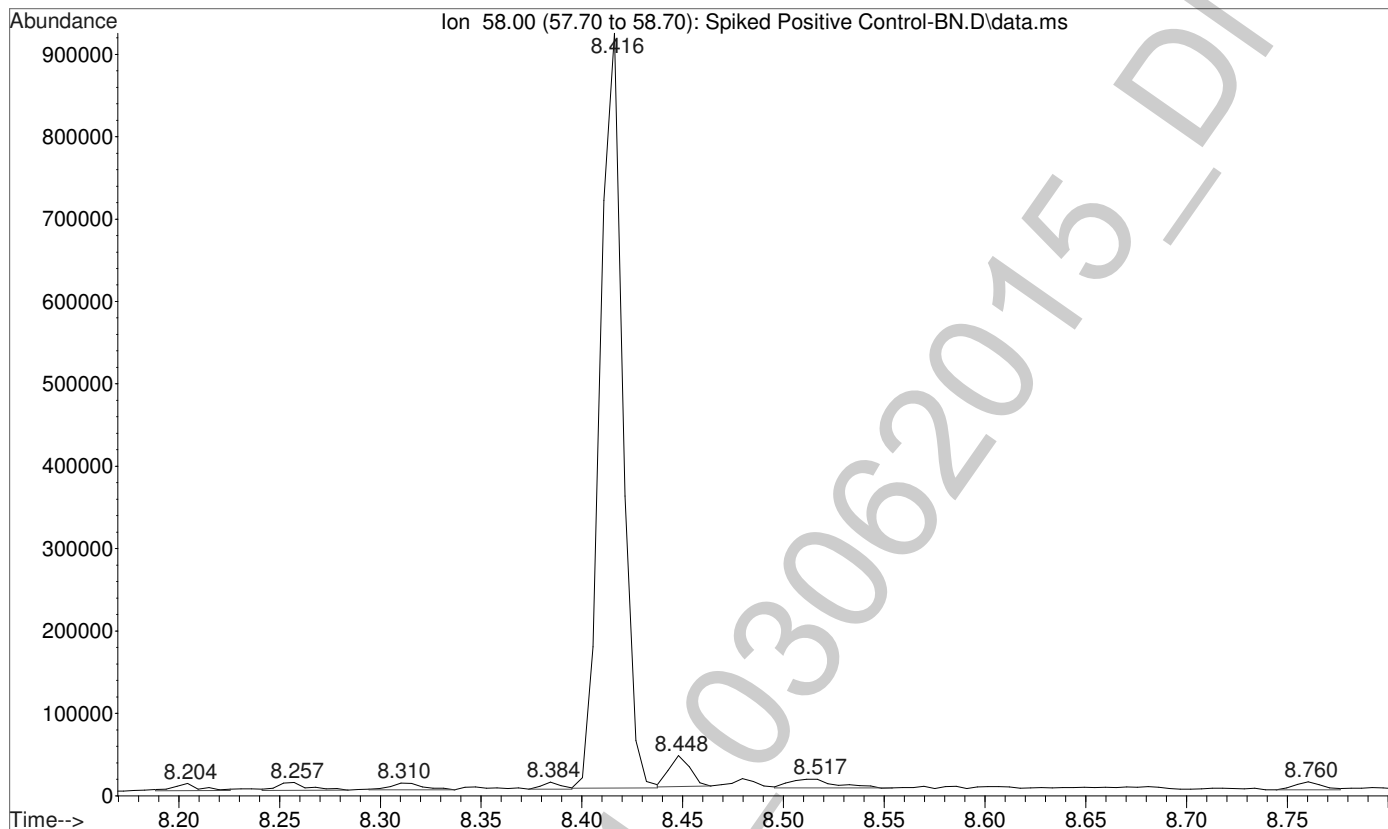



File :C:\gcms\1\data\Blood\030615BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 06 Mar 2015 09:33 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

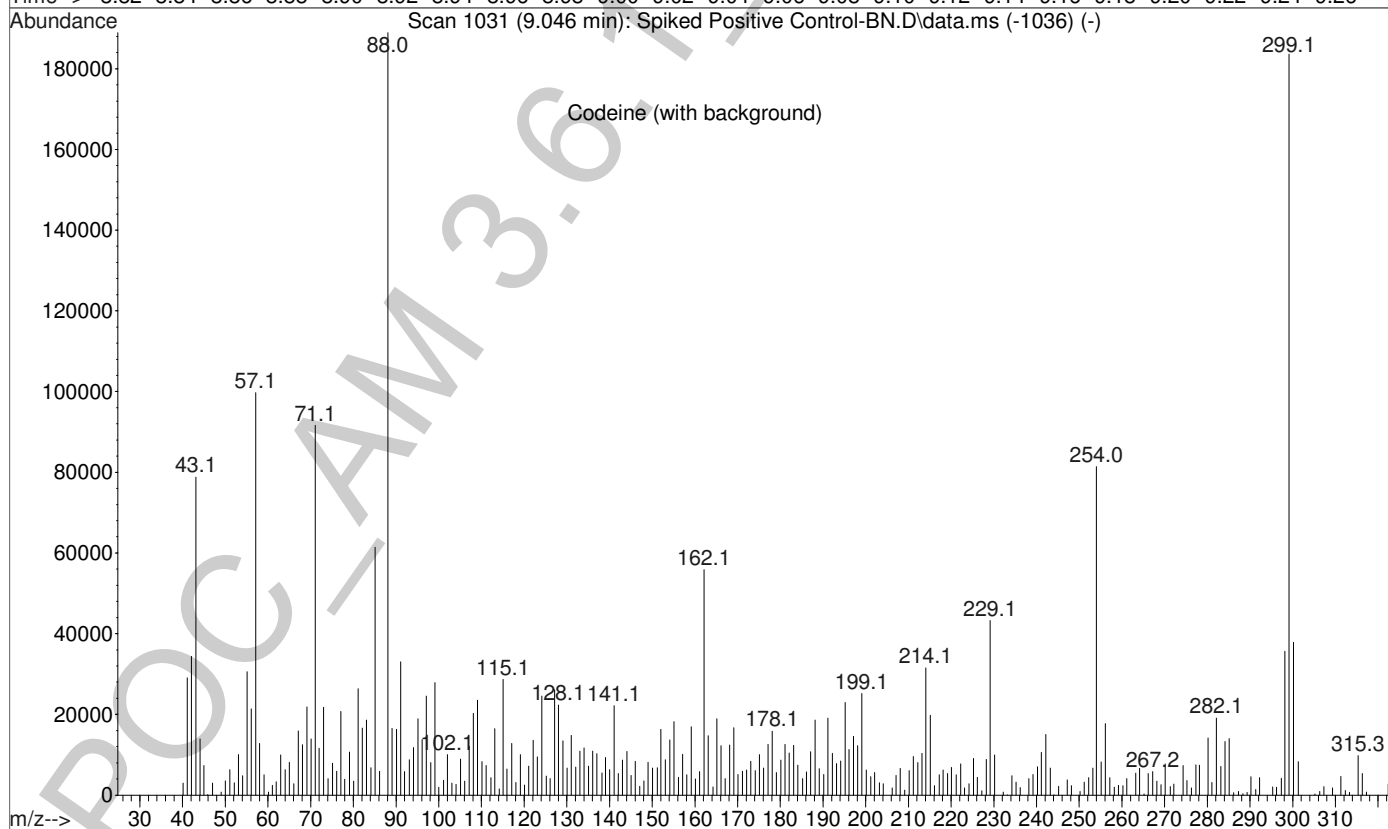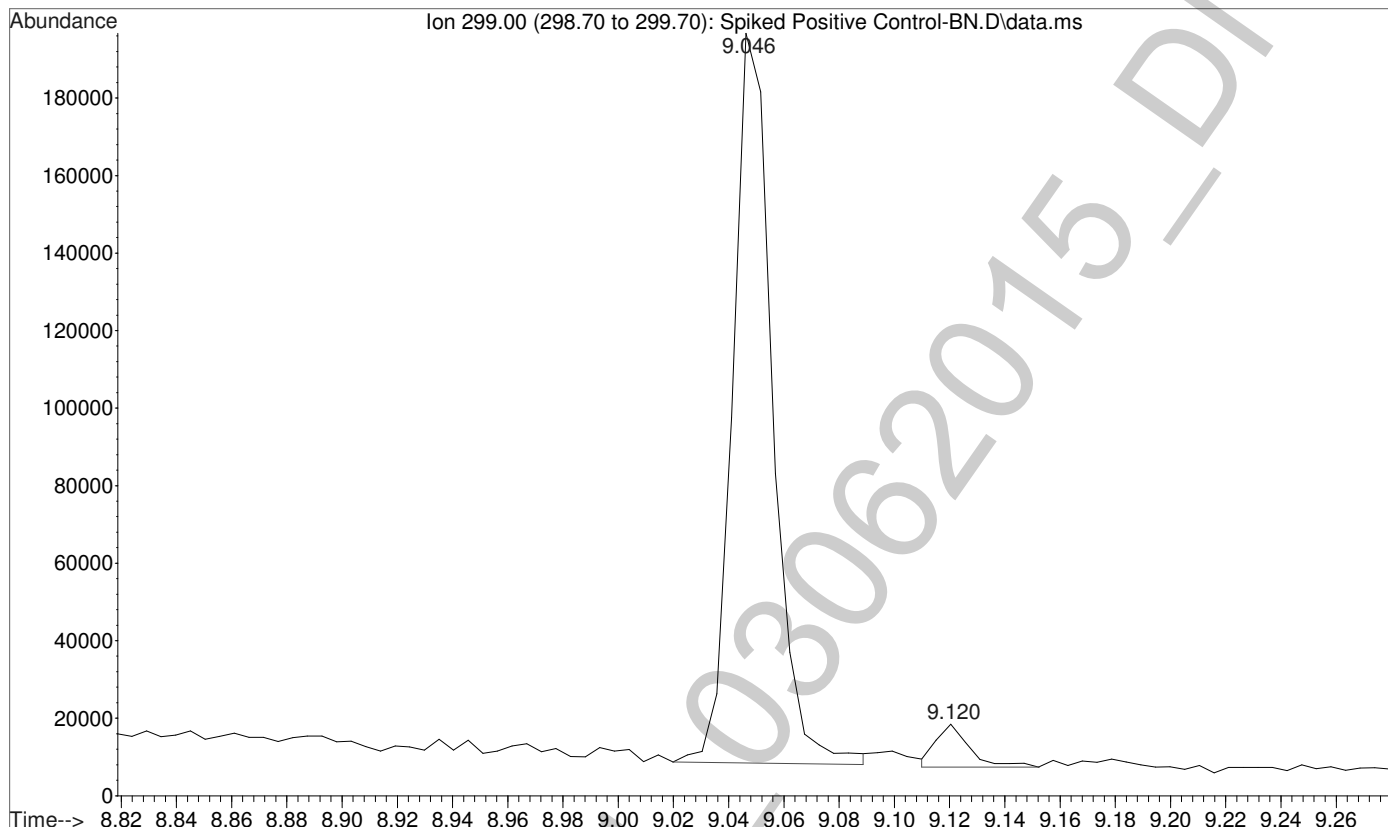

File :C:\gcms\1\data\Blood\030615BN\Spiked Positive Control-BN.D
Operator : 5LAB-C01\ISPuser
Acquired : 06 Mar 2015 09:33 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

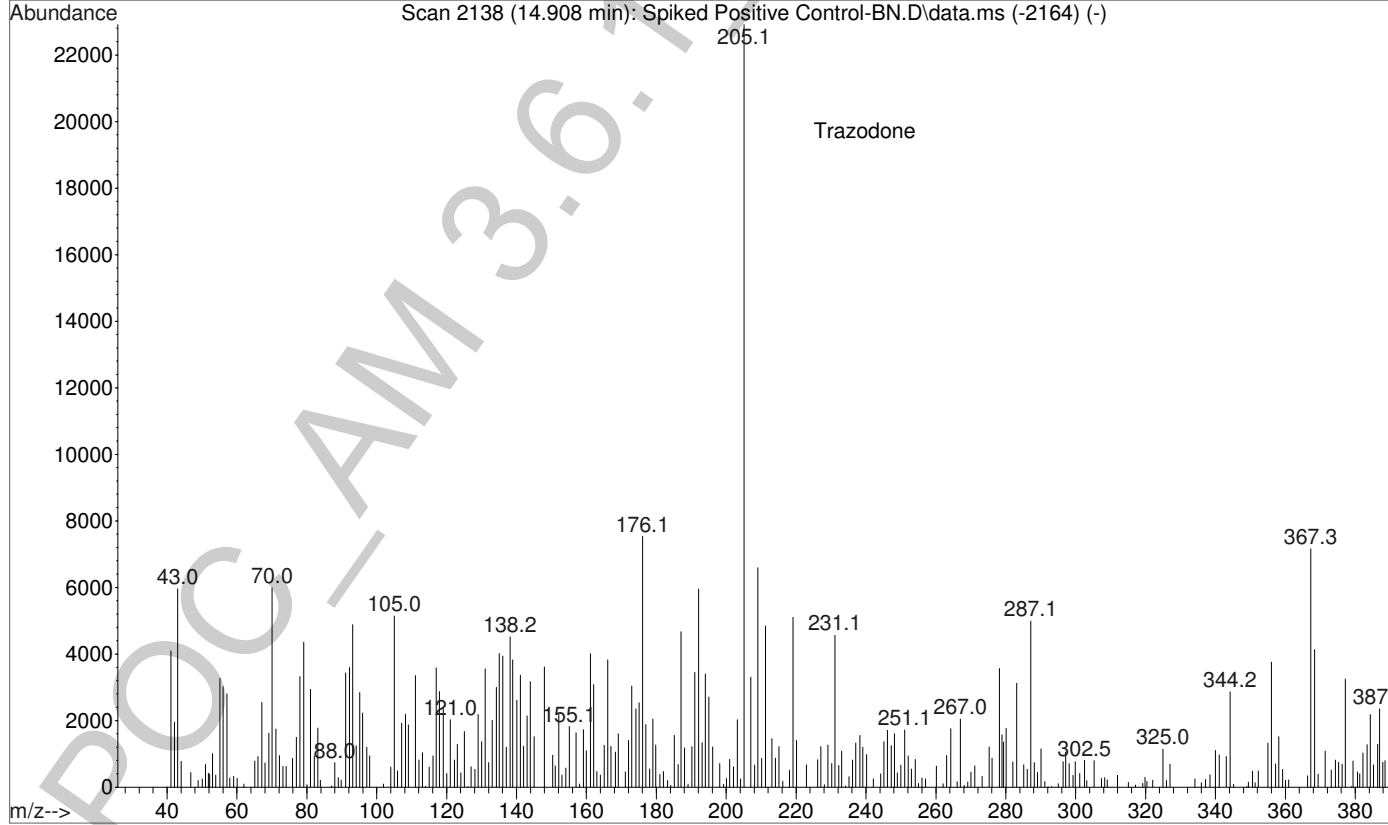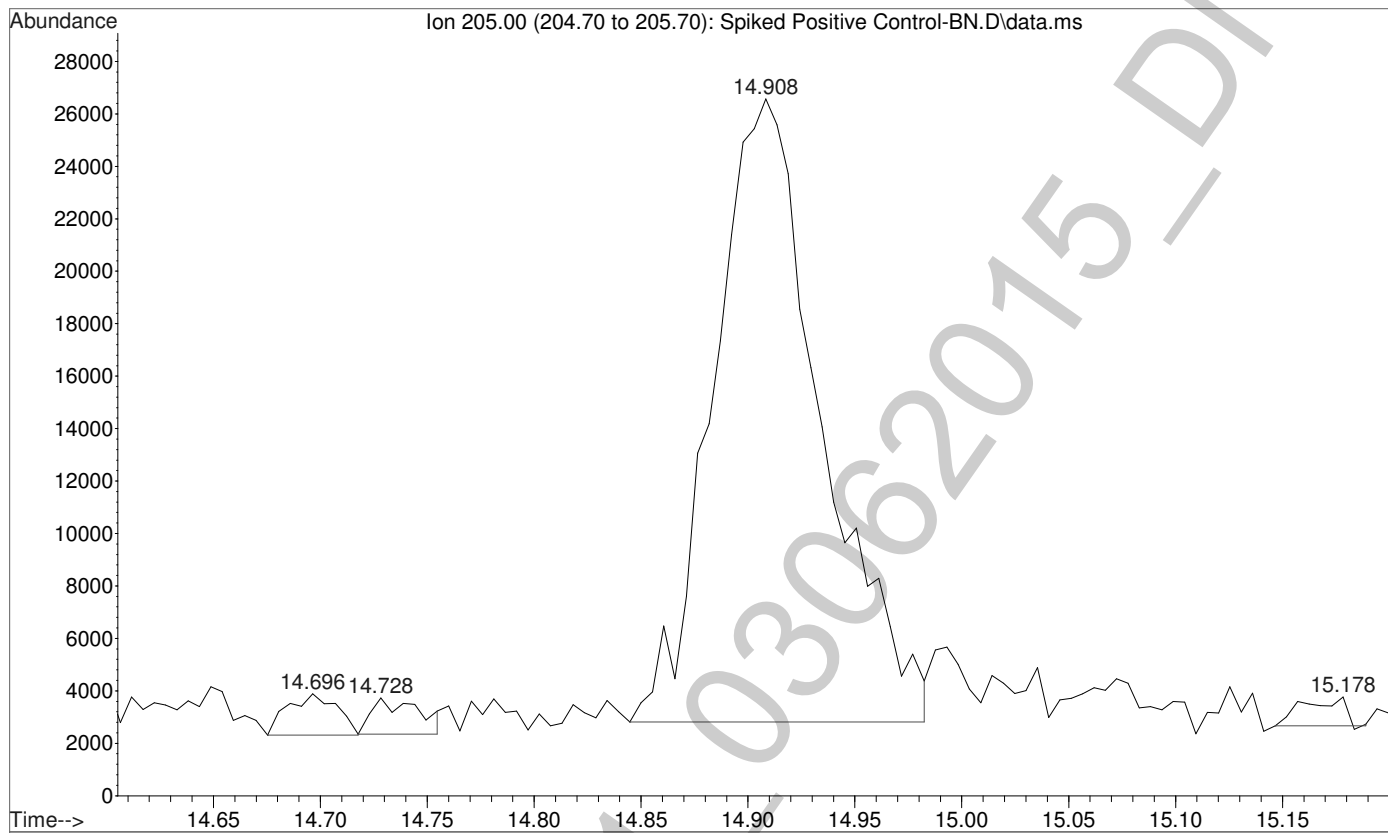

File :C:\gcms\1\data\Blood\030615BN\prbLK2.D
Operator : 5LAB-C01\ISPuser
Acquired : 06 Mar 2015 09:56 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Solvent Blank
Misc Info : Chloroform
Vial Number: 99

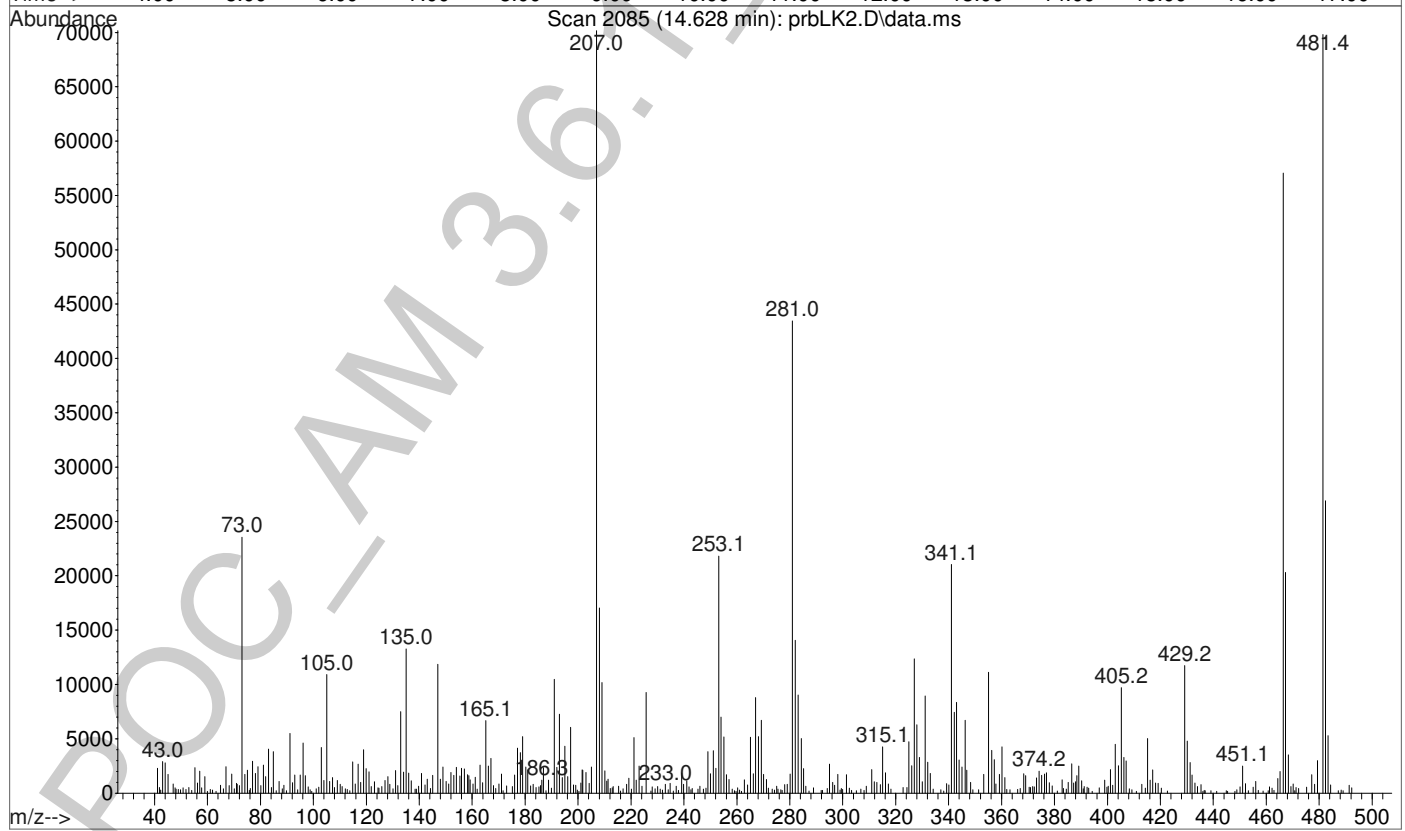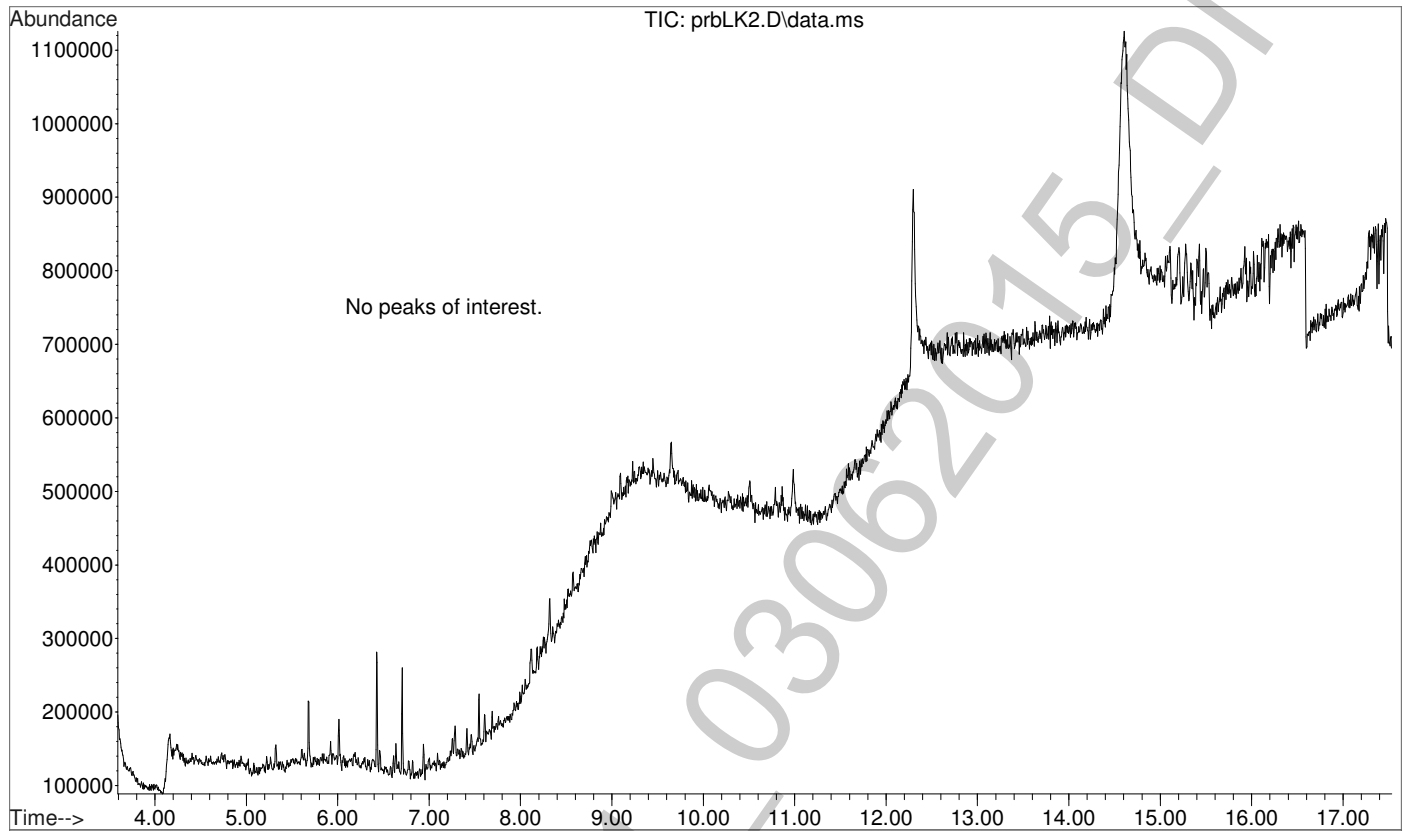

Analytical Method 3.6.1 & 3.6.7 QA Check List

Run Start Date: 03/06/15

Analyst: DND

(Long GC/MS temperature program)

Positive Control Compound List



- Methamphetamine
- Nicotine
- Meperidine
- Caffeine
- Diphenhydramine
- Lidocaine
- PCP
- Methadone
- Amitriptyline
- Codeine
- Trazodone

Internal Standards


- Benzphetamine
- Papaverine

Optional back extraction **not** performed.
Samples reconstituted in methanol.



File :C:\gcms\1\data\Blood\030615BN\Reinjection Longer GC Method\P
... rerun Solvent Blankr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 06 Mar 2015 10:19 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Pre-run Solvent Blank
Misc Info : Chloroform

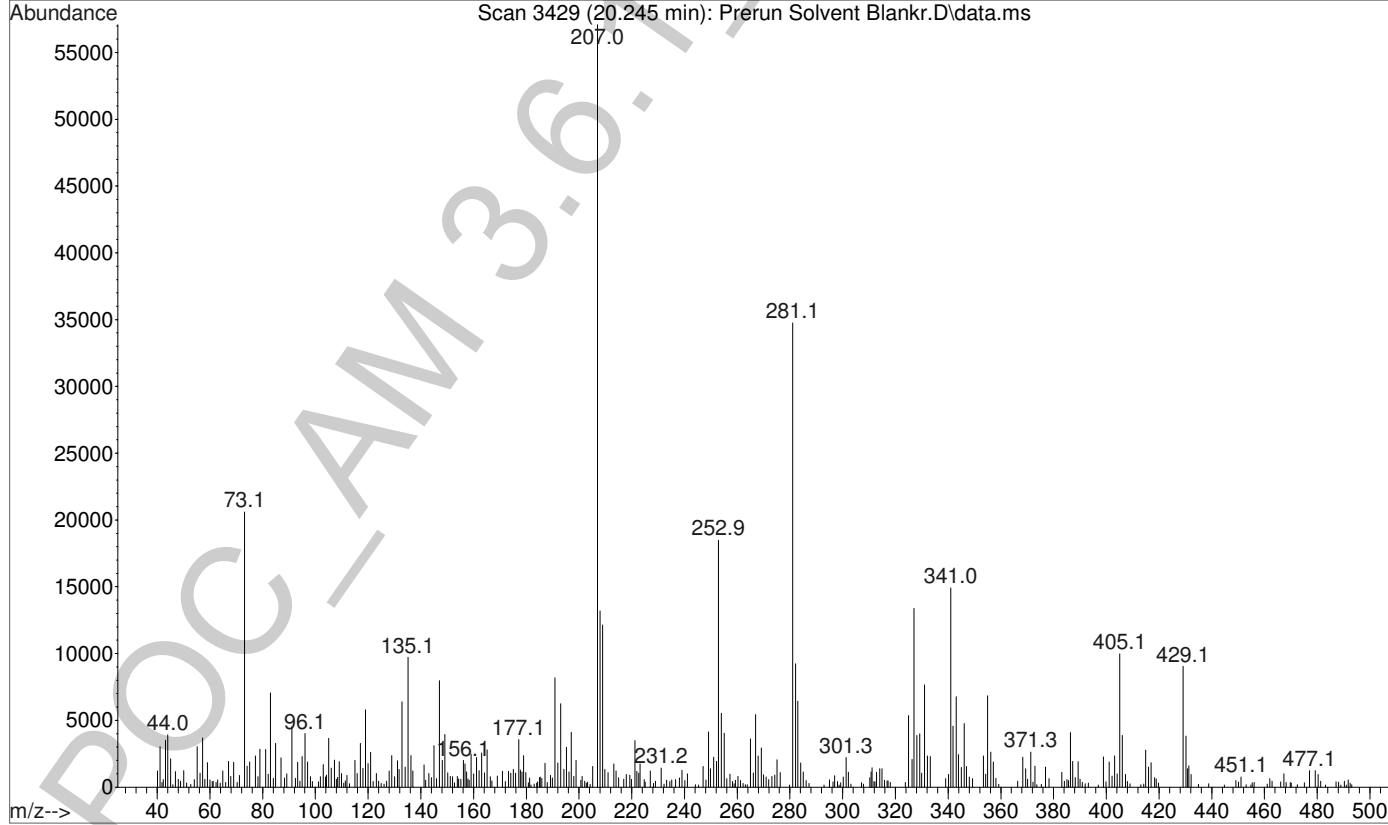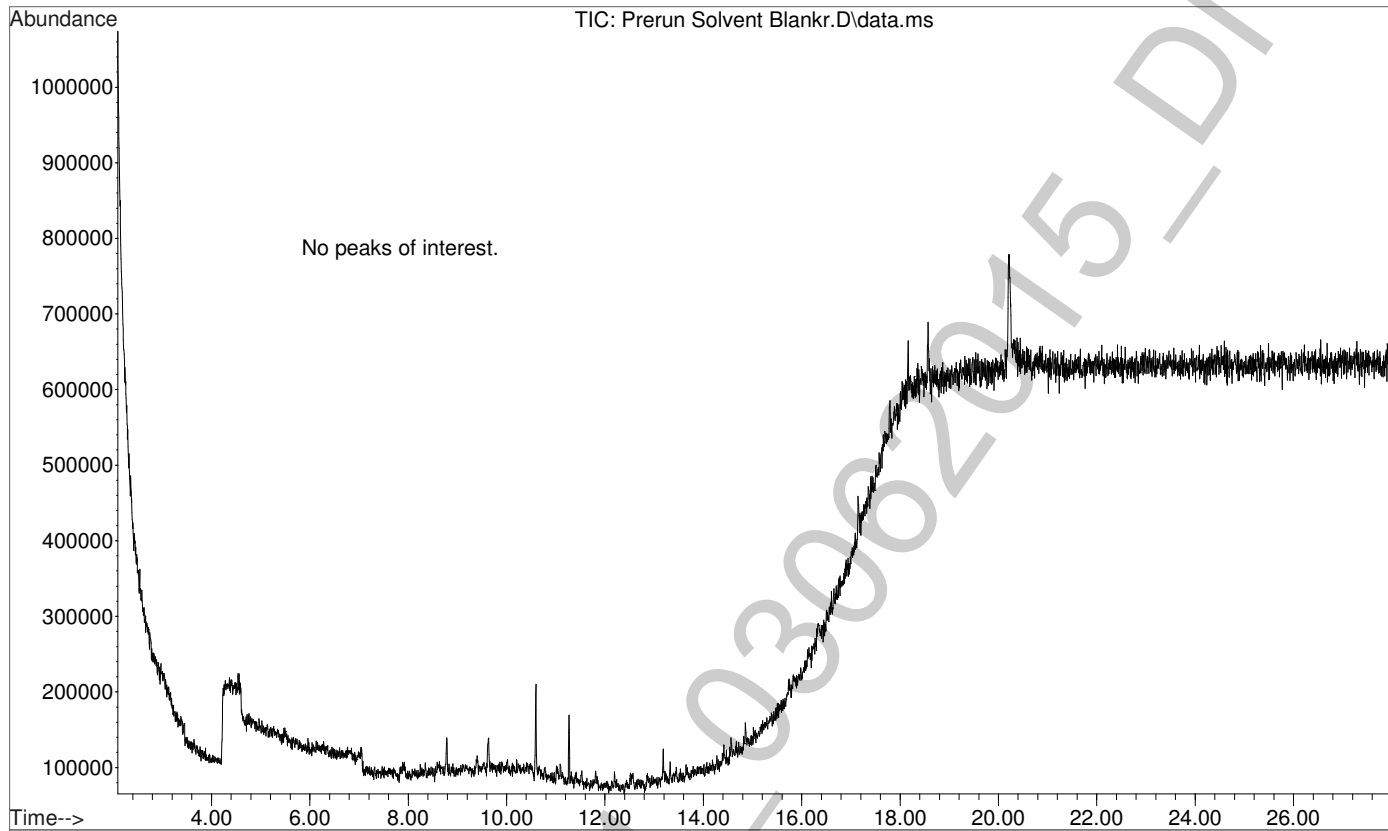



File :C:\gcms\1\data\Blood\030615BN\Reinjection Longer GC Method\N
... egative Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 06 Mar 2015 10:53 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Negative Control - Utak Lot B0130
Misc Info : Analytical Method 3.6.1

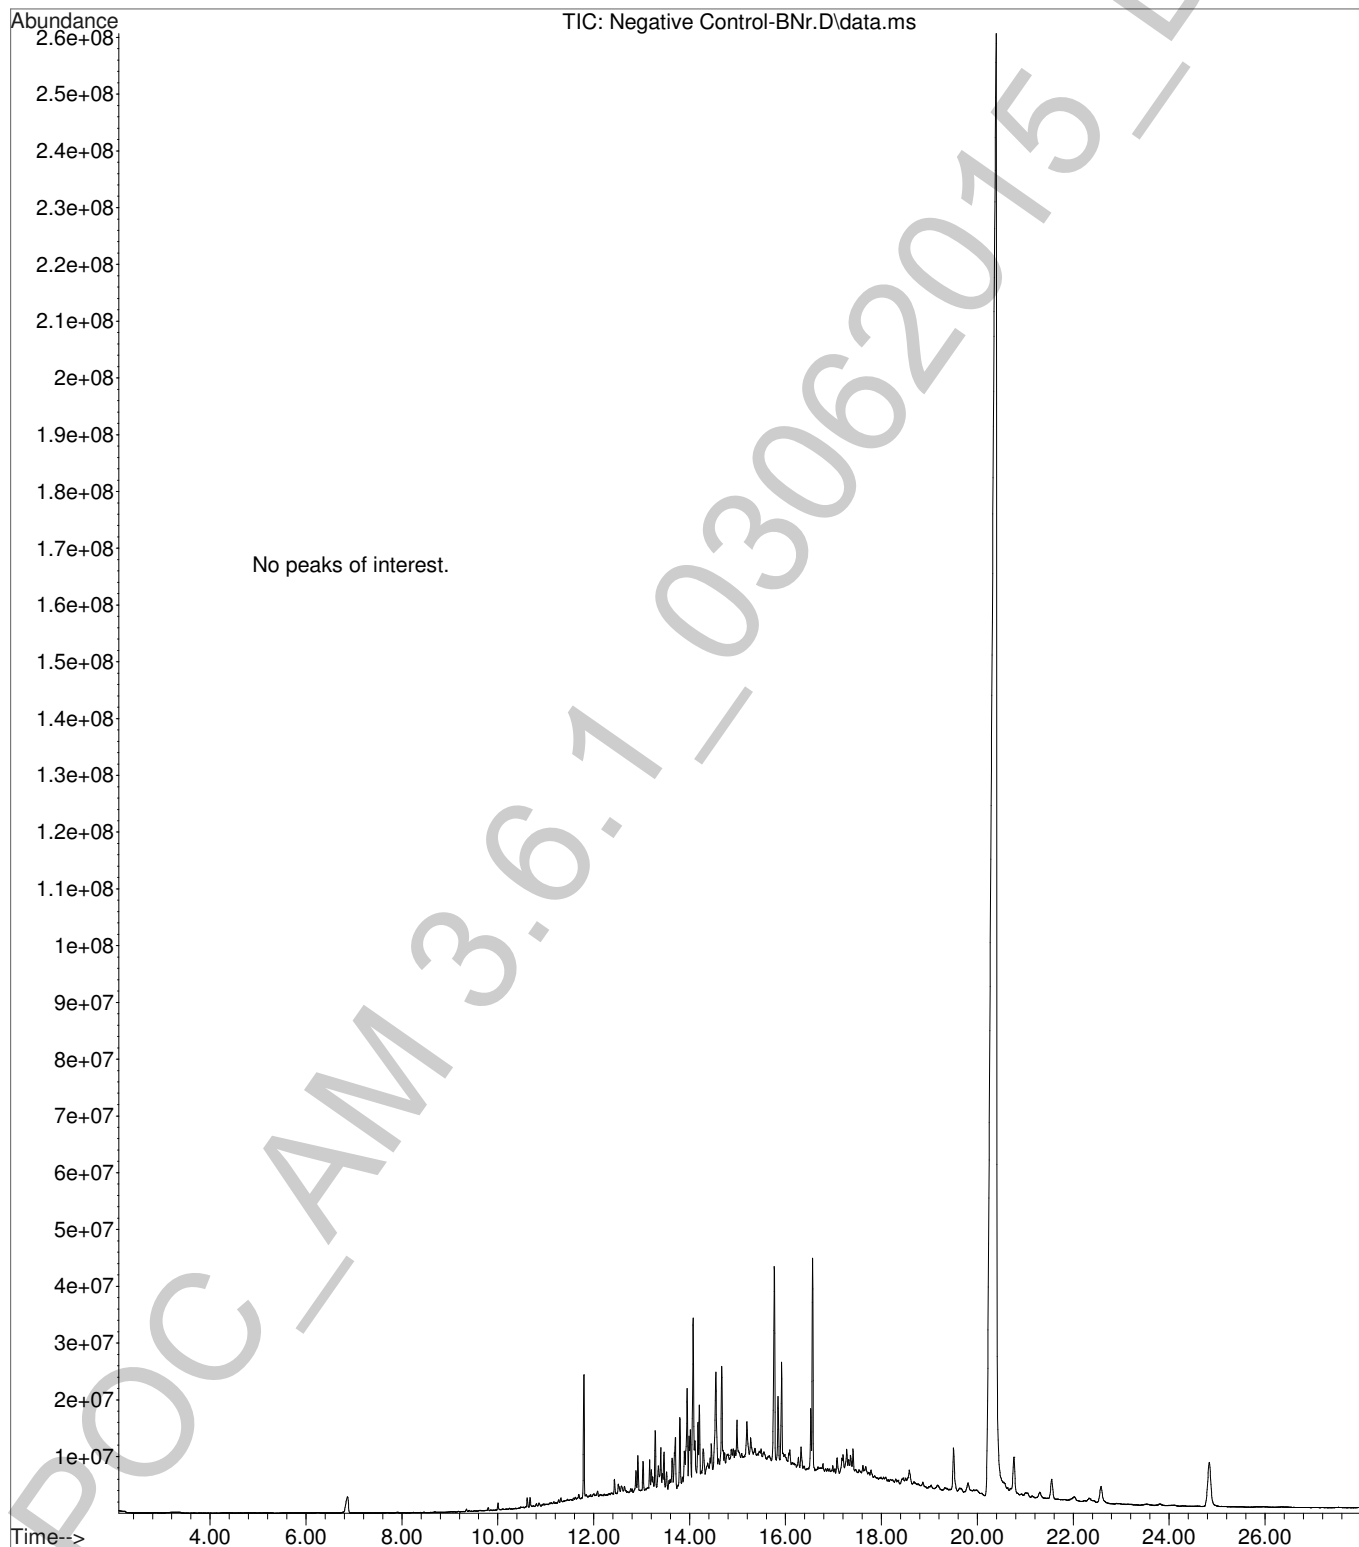

File :C:\gcms\1\data\Blood\030615BN\Reinjection Longer GC Method\N
... egative Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 06 Mar 2015 10:53 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Negative Control - Utak Lot B0130
Misc Info : Analytical Method 3.6.1

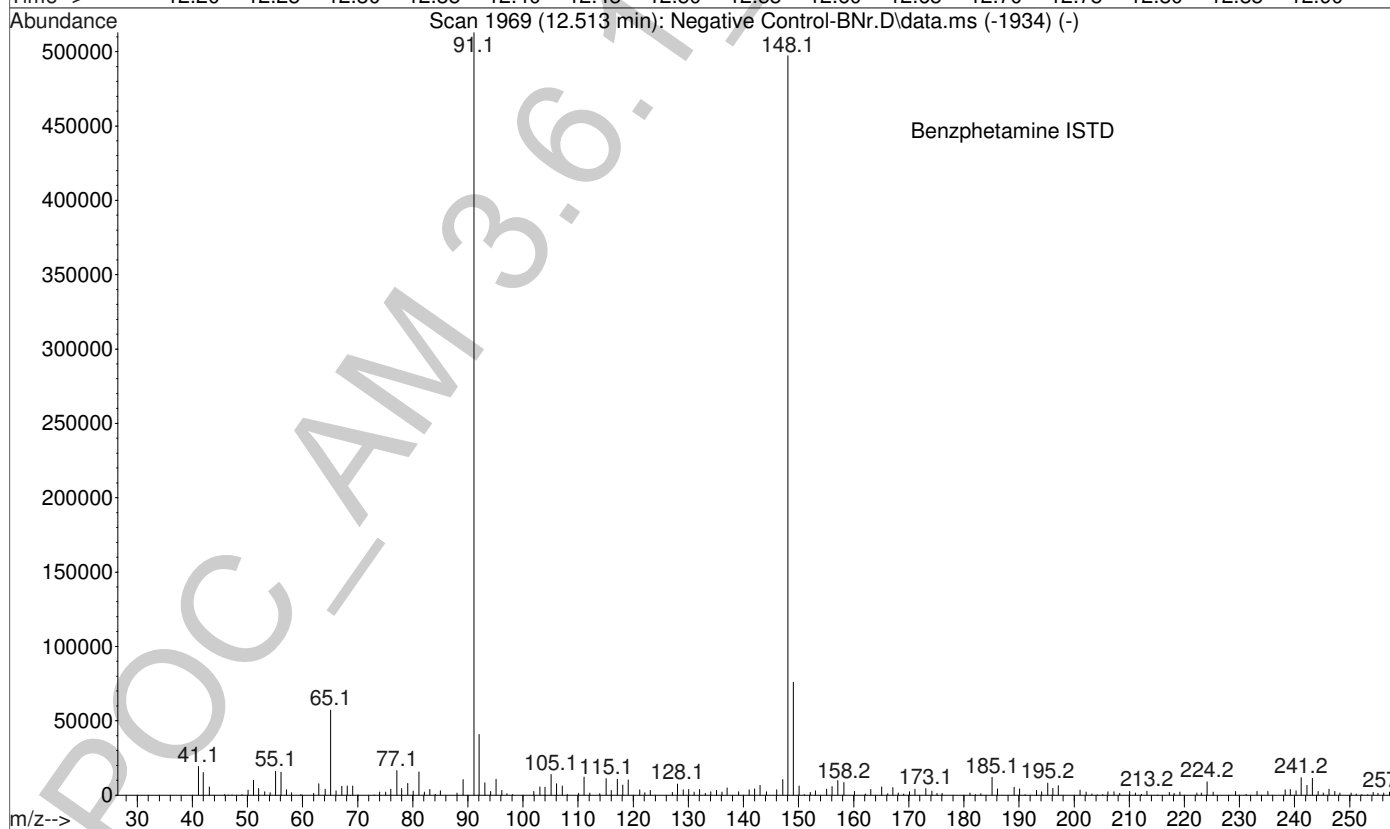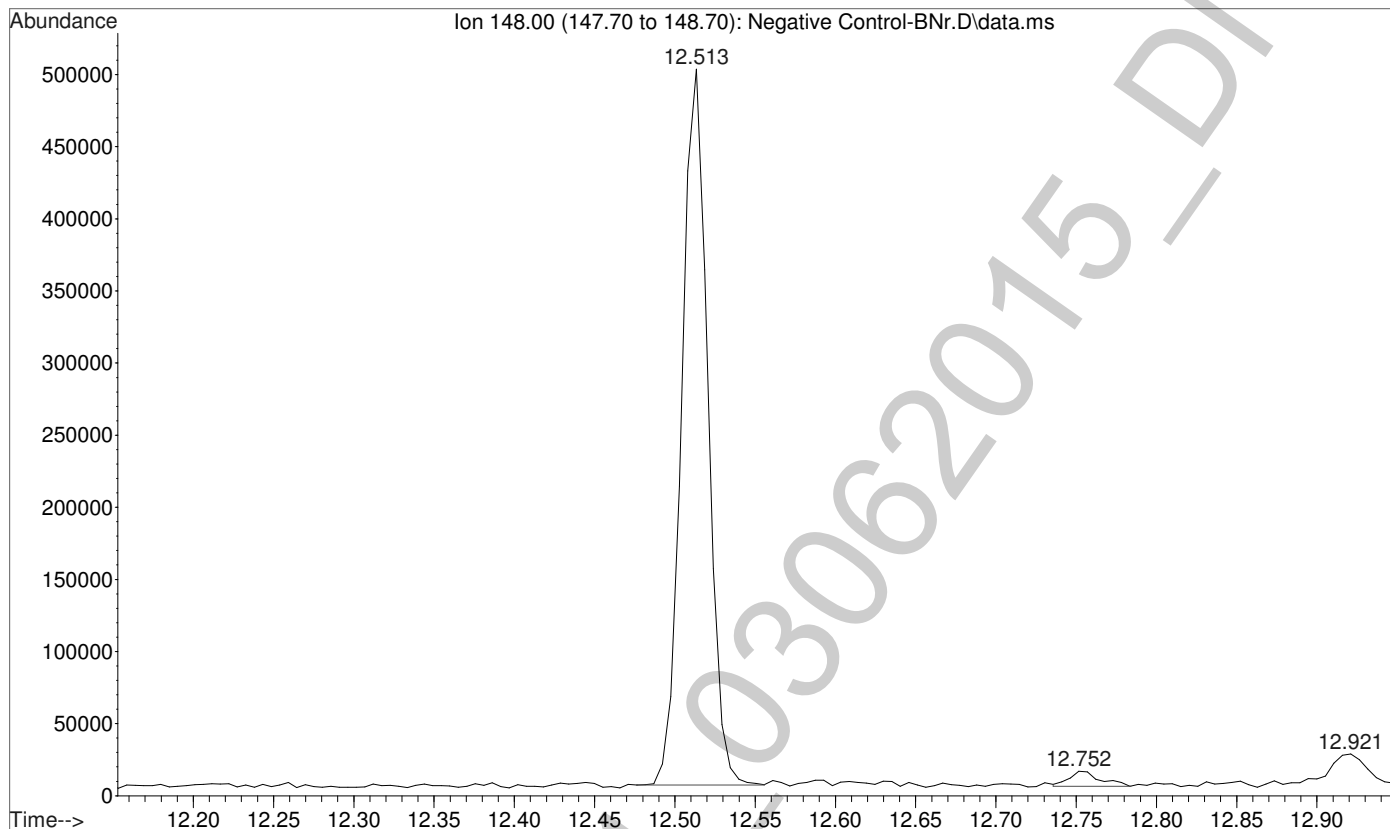


File :C:\gcms\1\data\Blood\030615BN\Reinjection Longer GC Method\N
... egative Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 06 Mar 2015 10:53 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Negative Control - Utak Lot B0130
Misc Info : Analytical Method 3.6.1

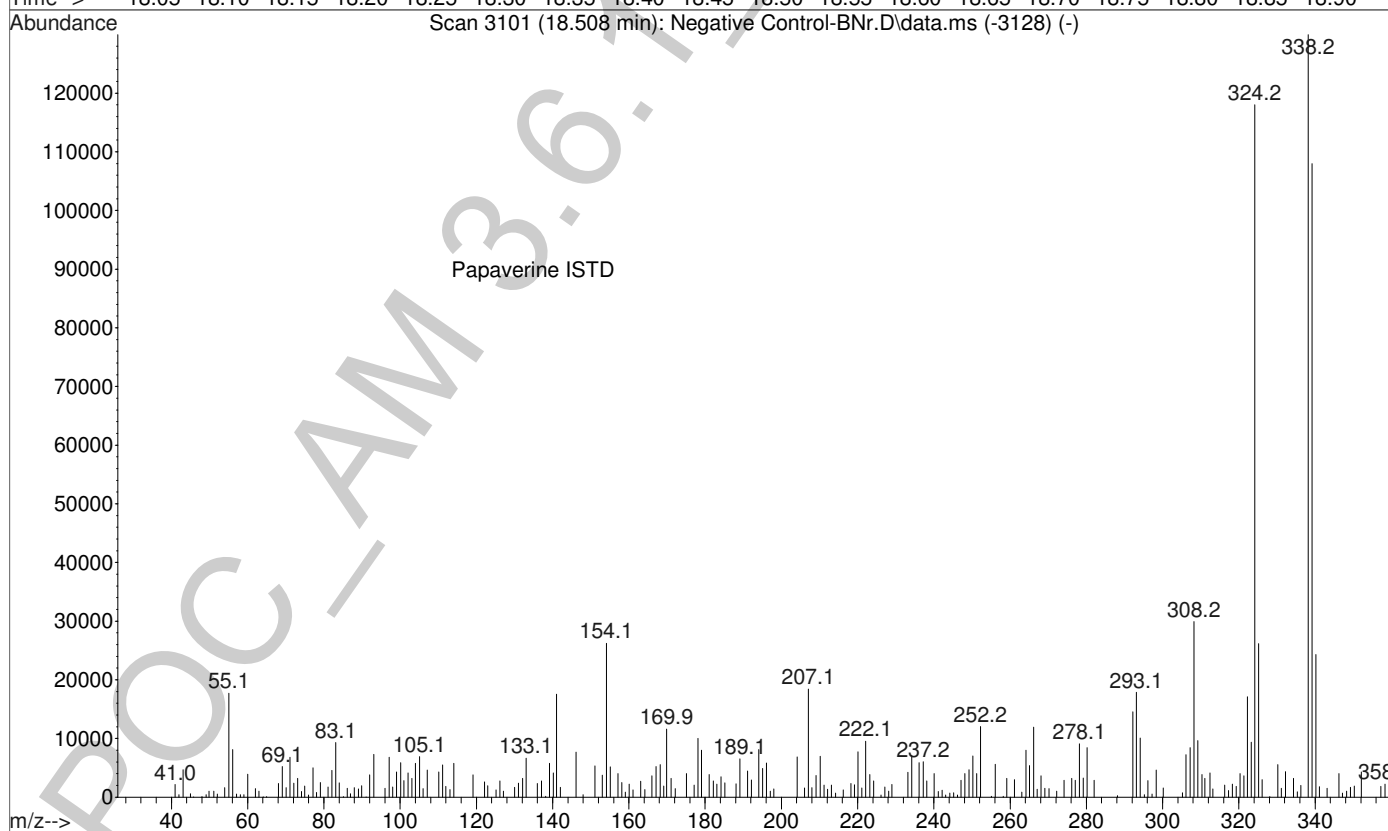
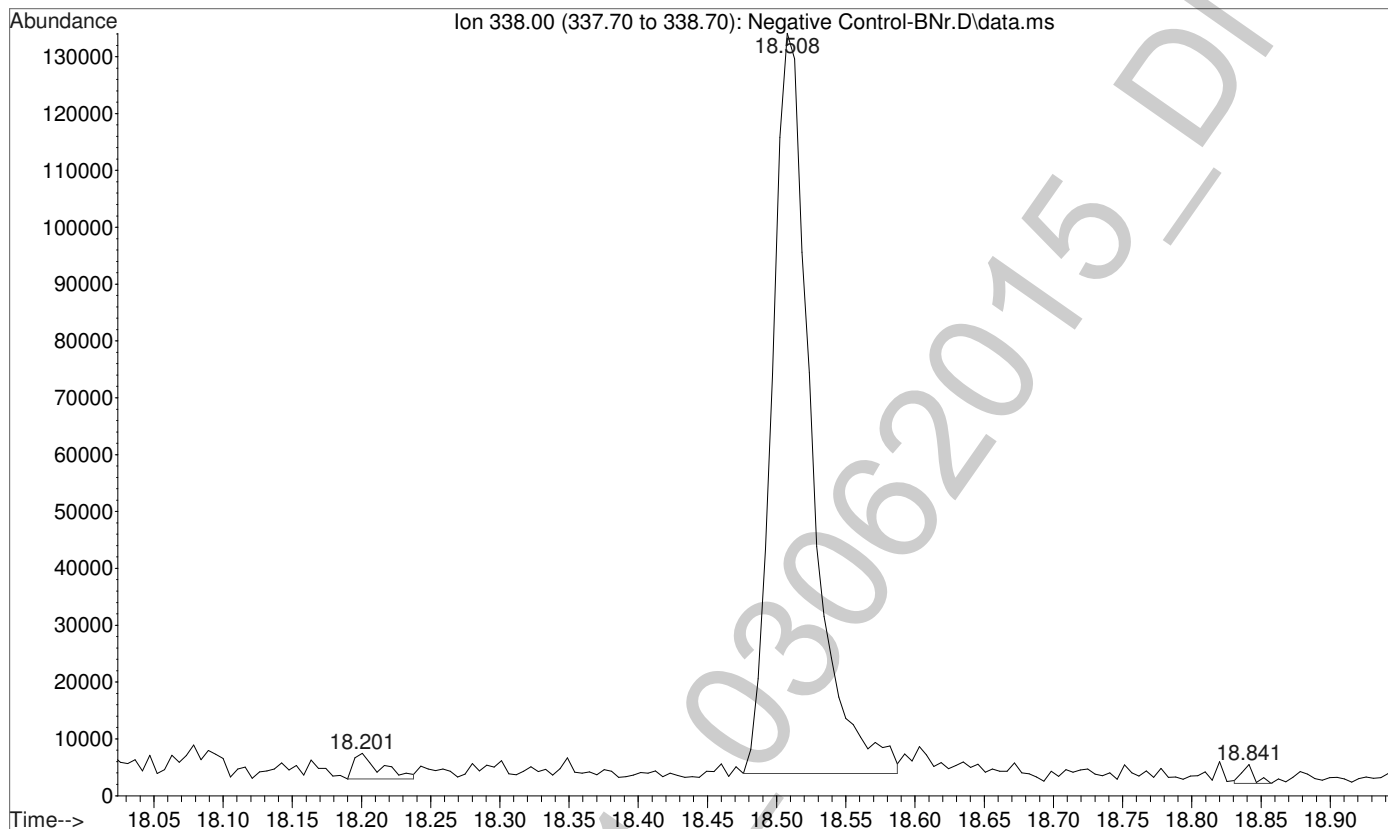






File :C:\gcms\1\data\Blood\030615BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 06 Mar 2015 11:27 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

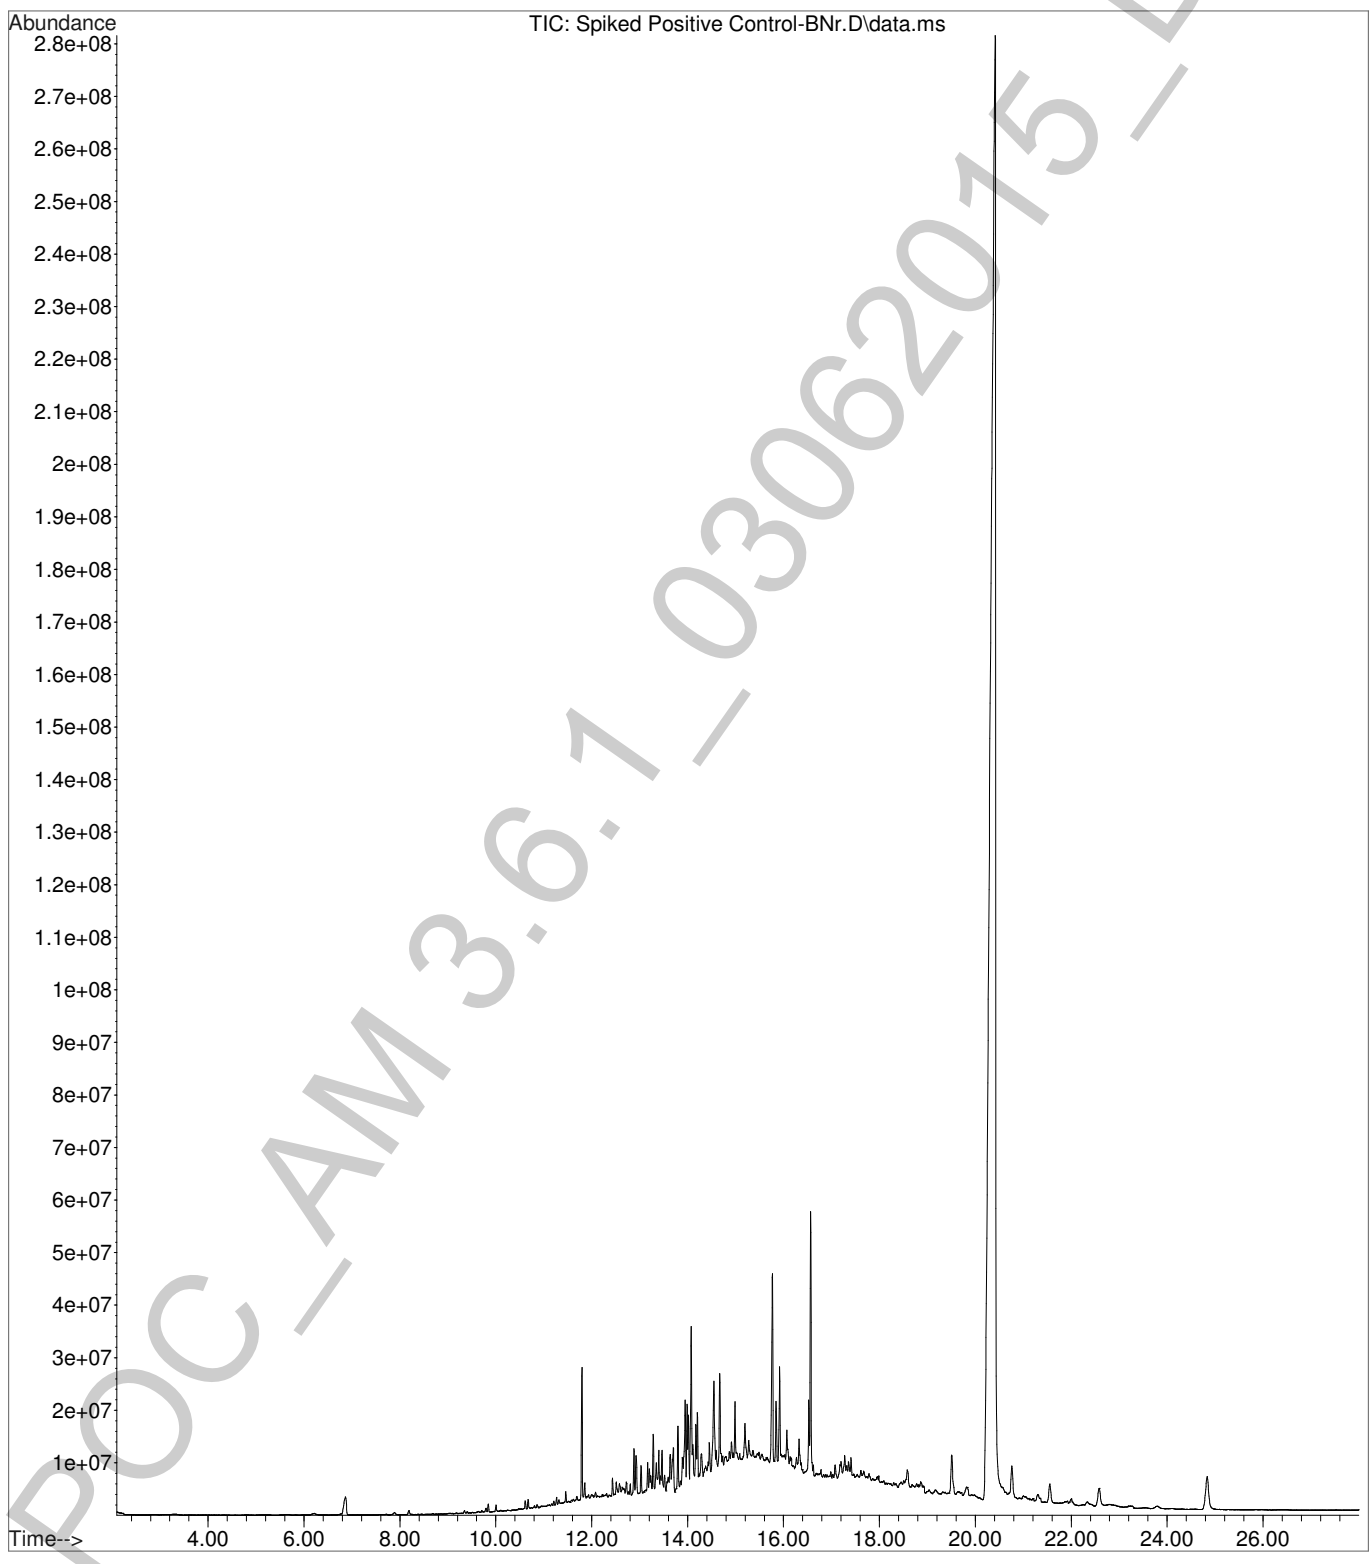



File :C:\gcms\1\data\Blood\030615BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 06 Mar 2015 11:27 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

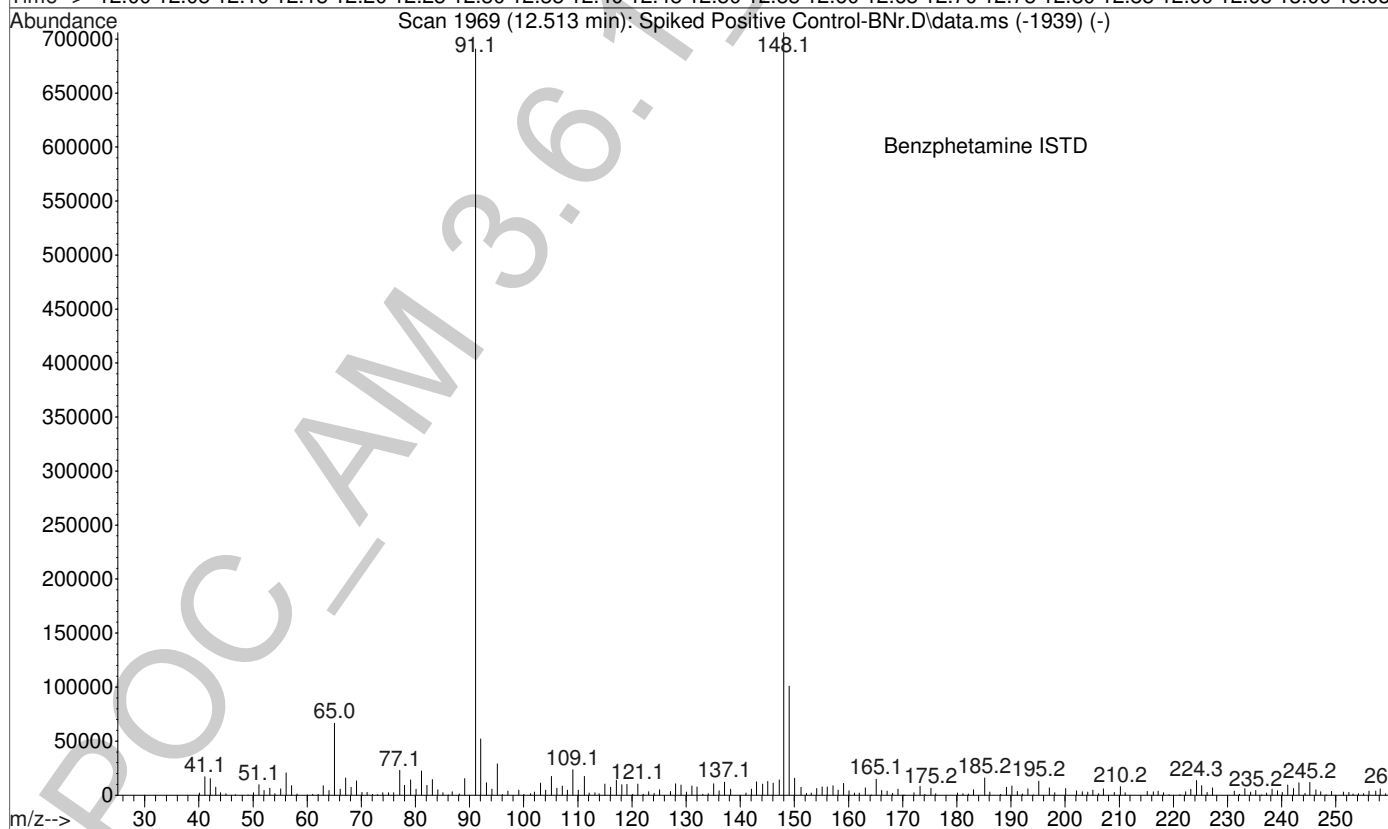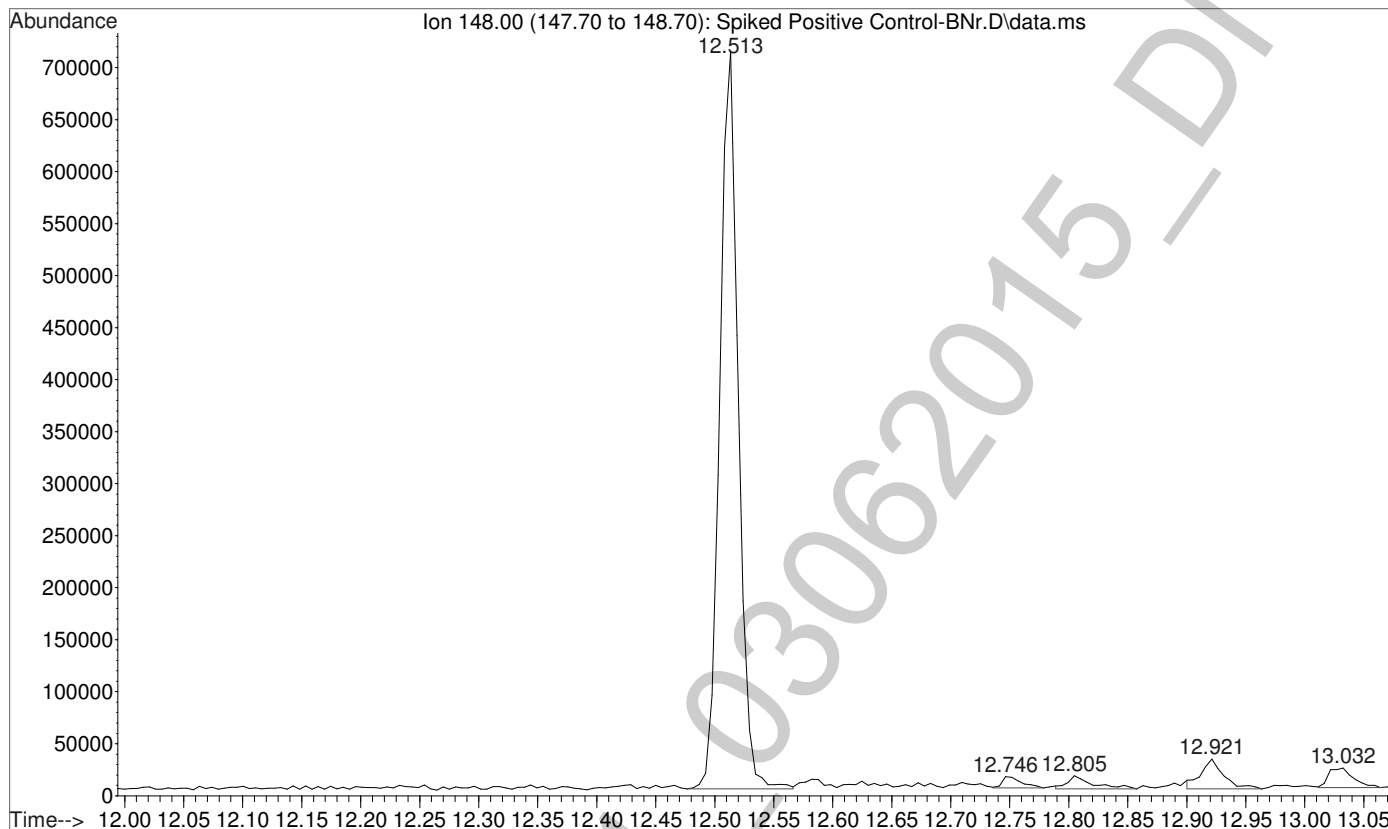



File :C:\gcms\1\data\Blood\030615BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 06 Mar 2015 11:27 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

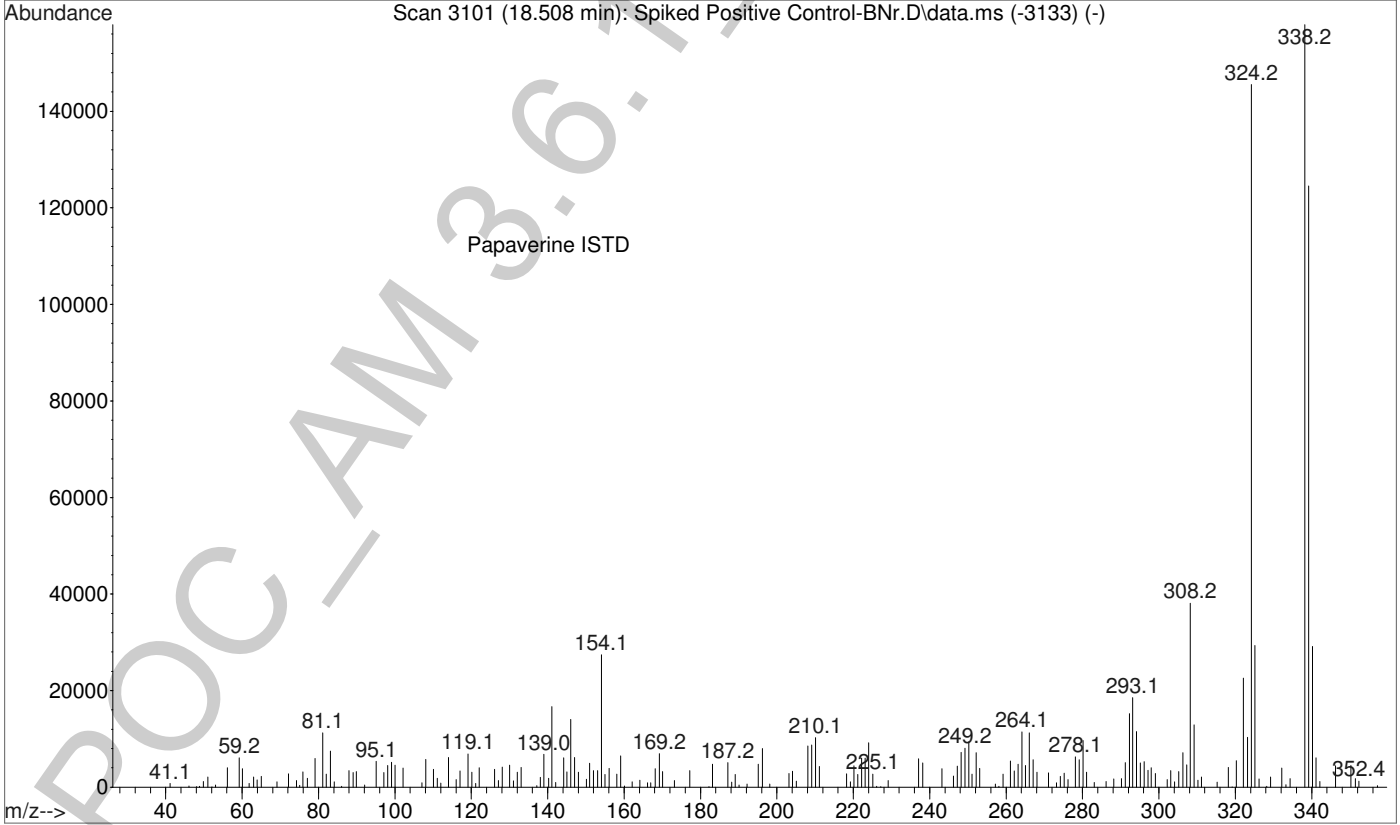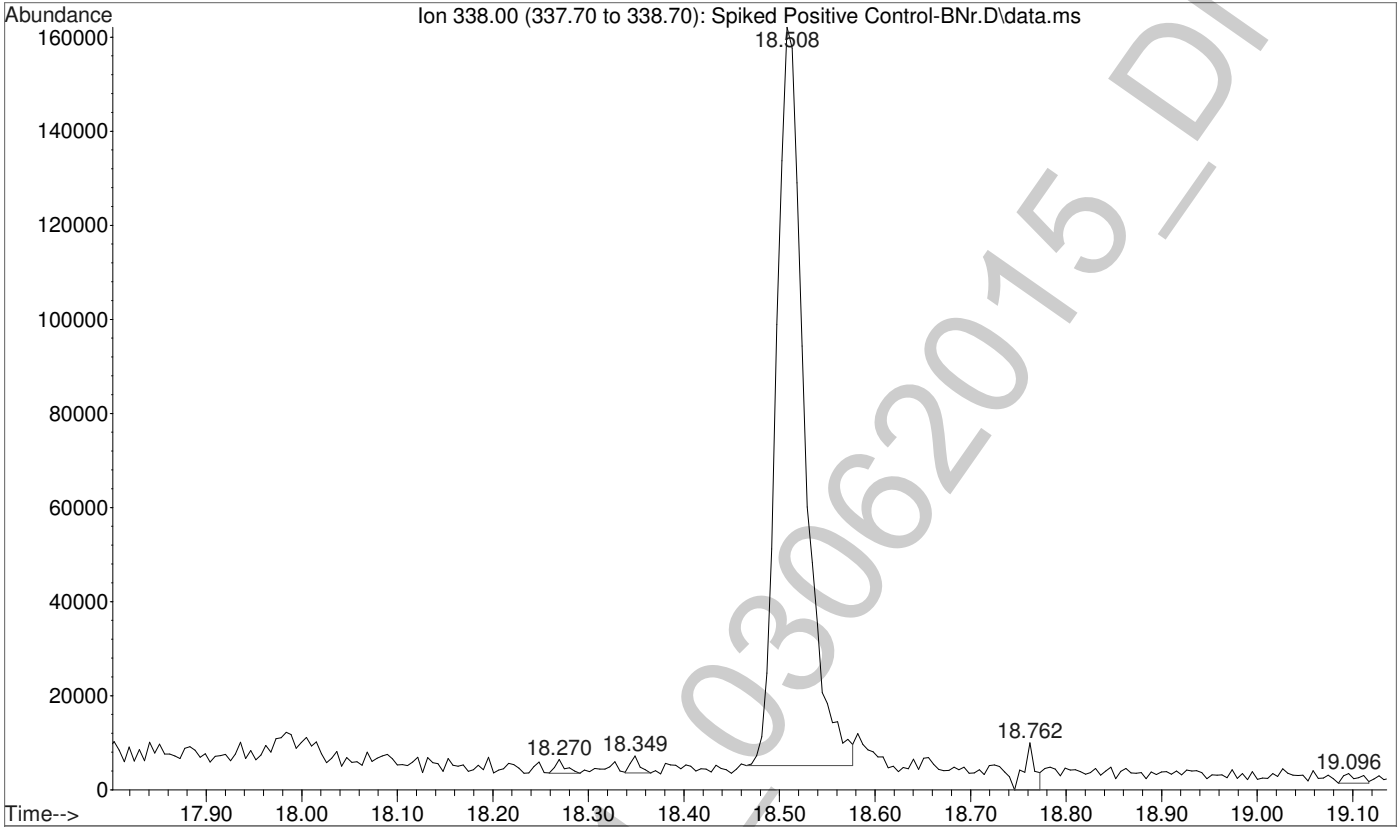



File :C:\gcms\1\data\Blood\030615BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 06 Mar 2015 11:27 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

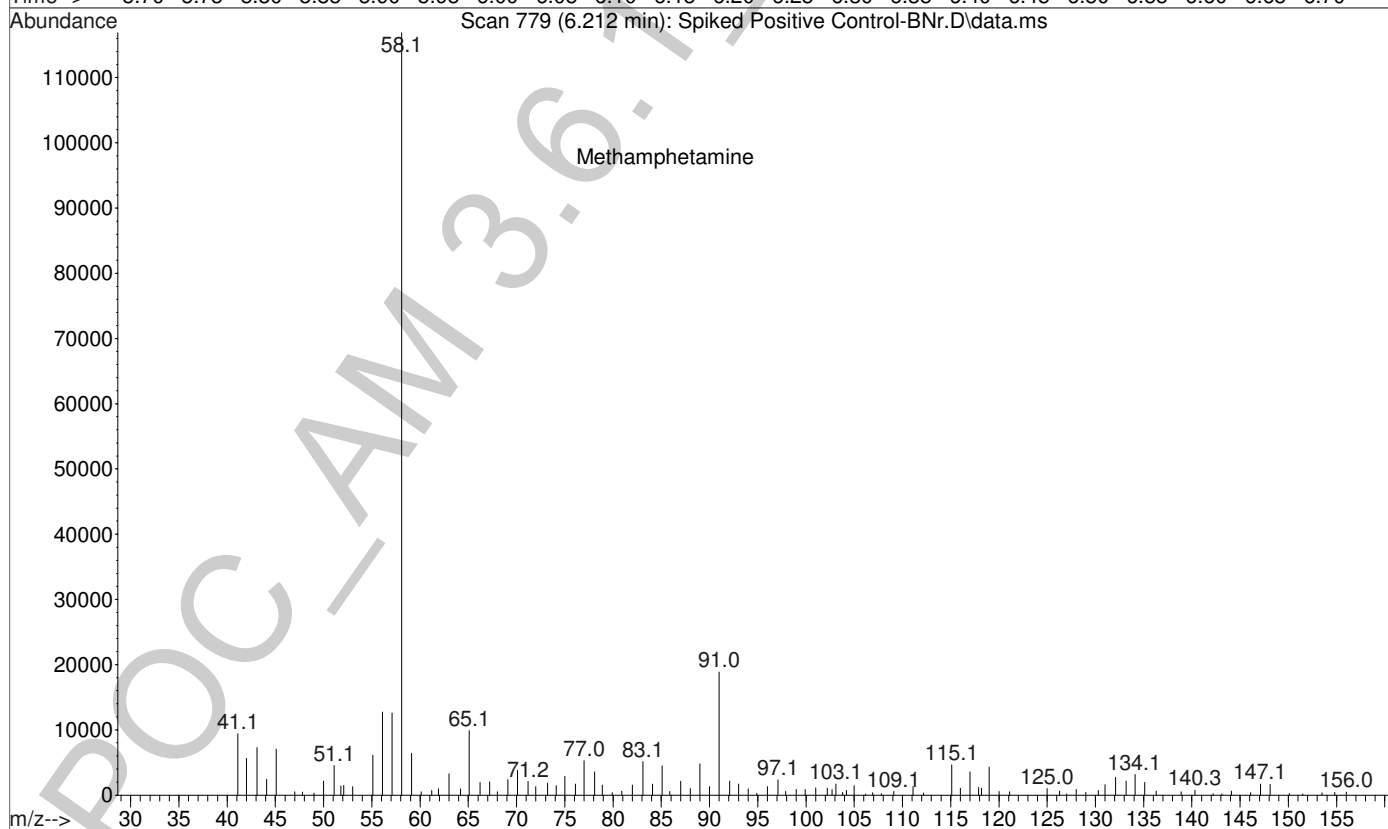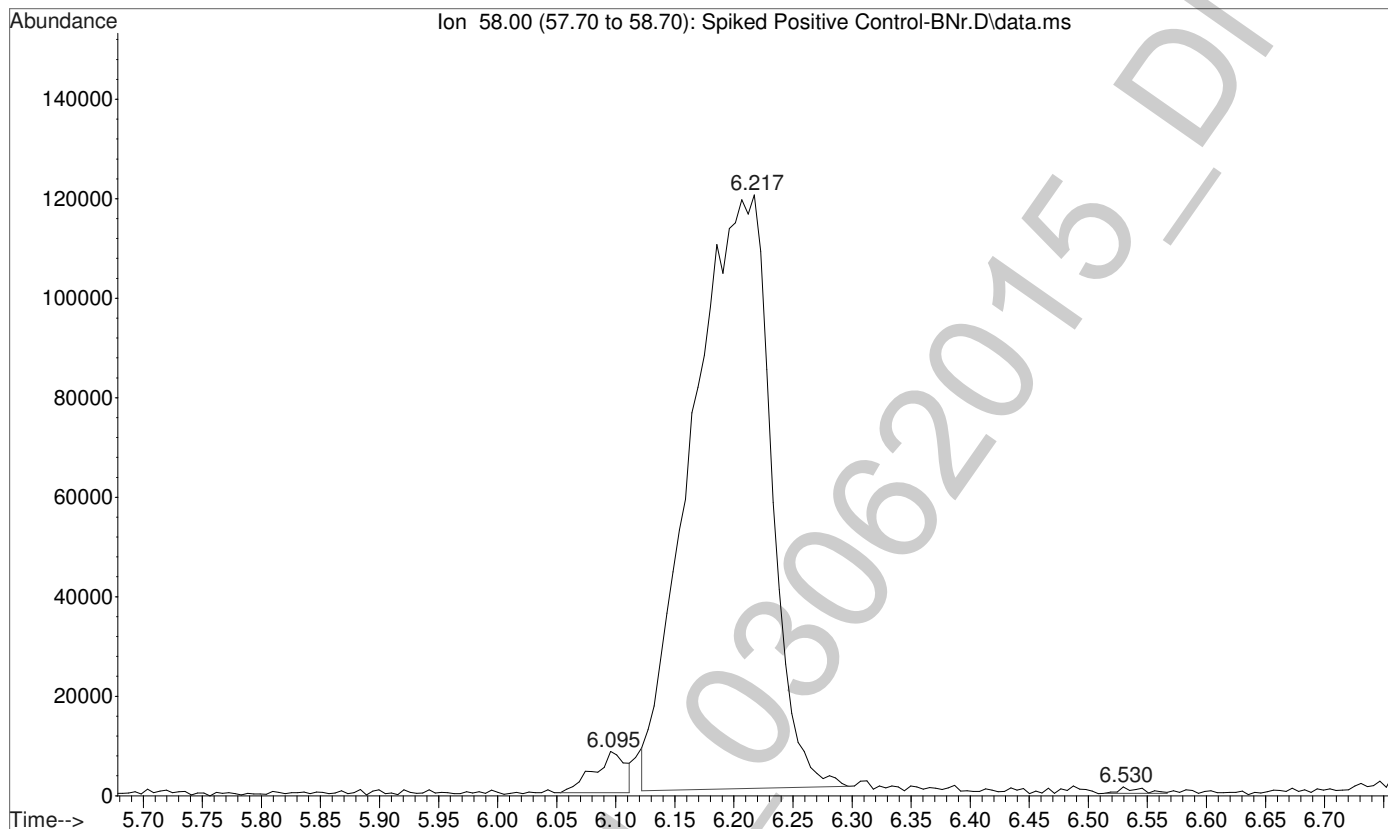



File :C:\gcms\1\data\Blood\030615BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 06 Mar 2015 11:27 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

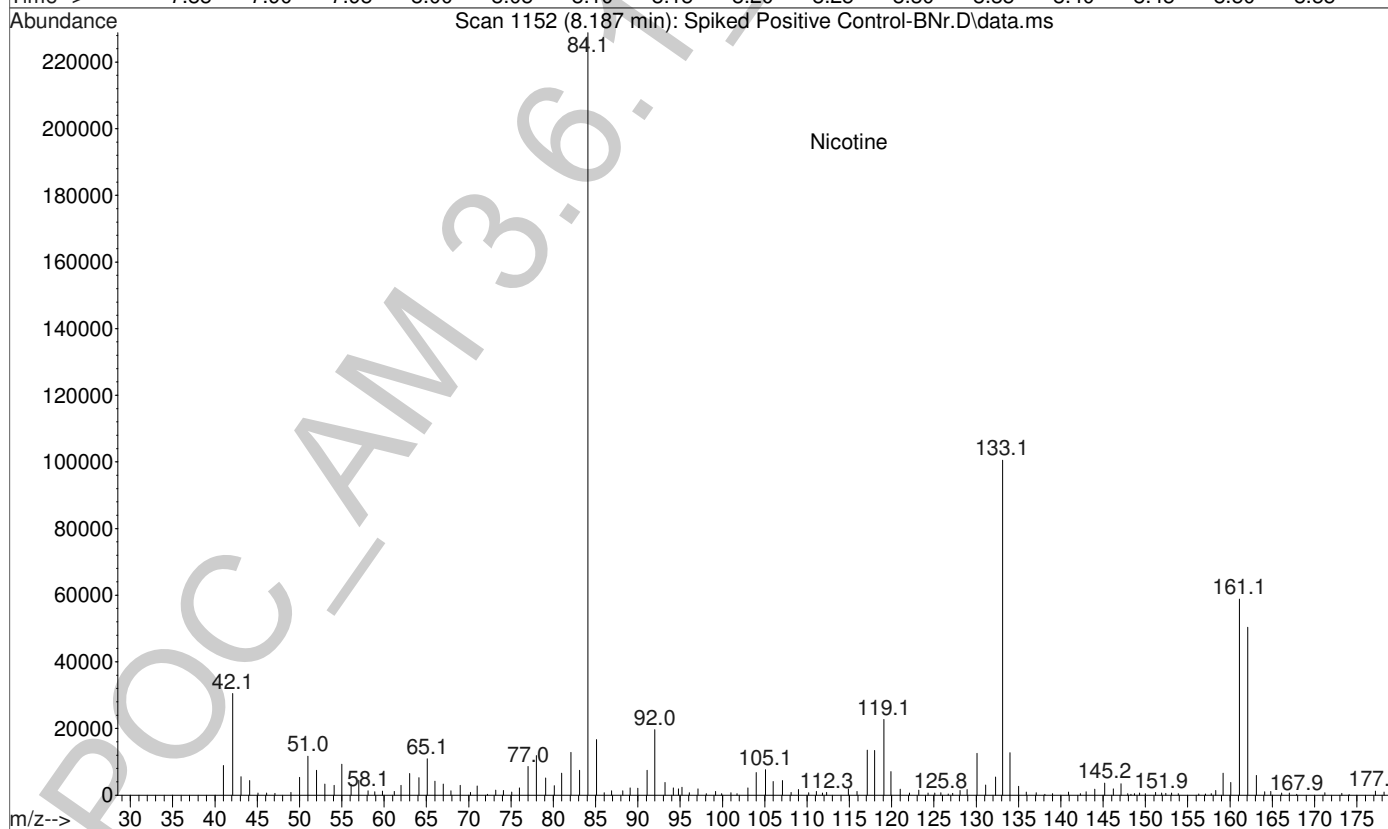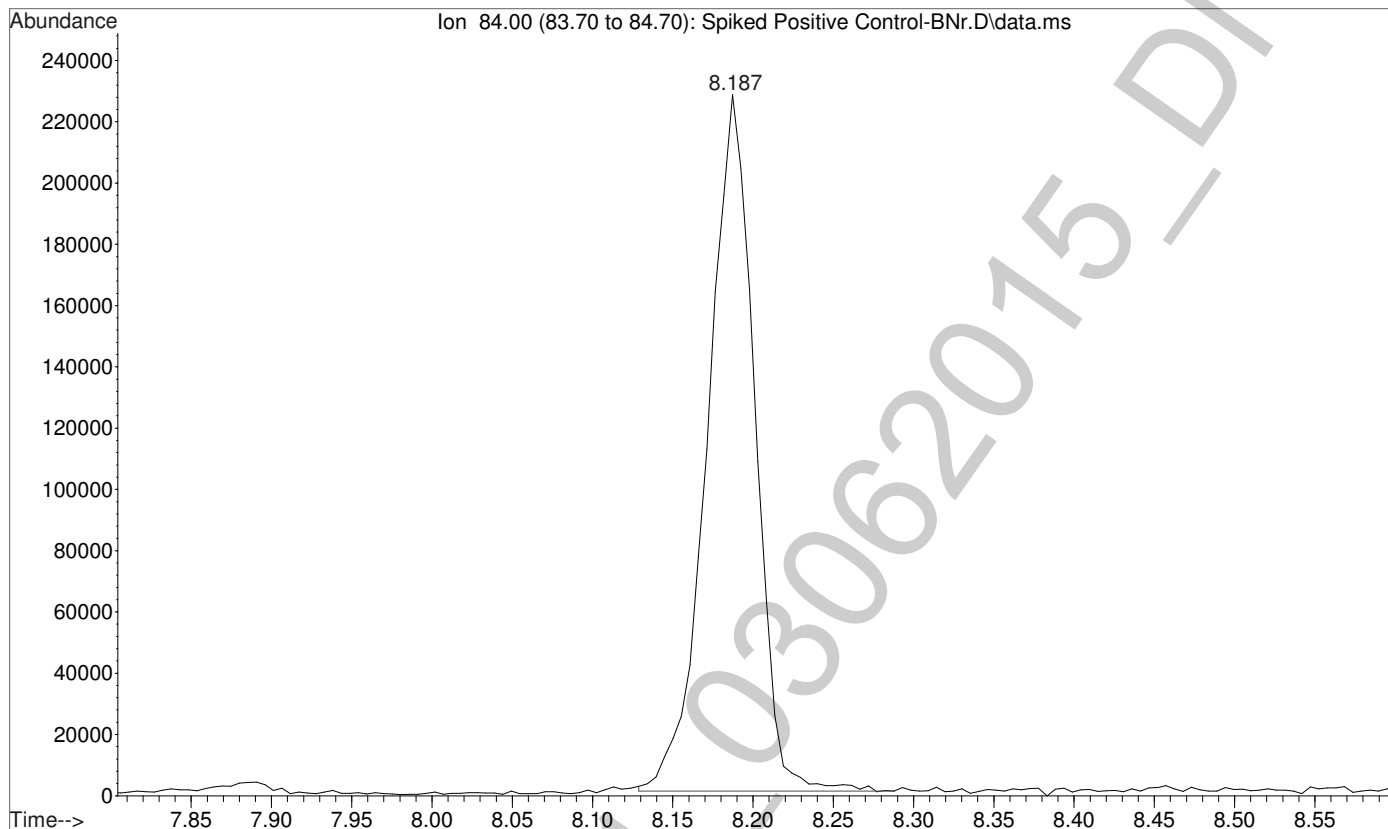



File :C:\gcms\1\data\Blood\030615BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 06 Mar 2015 11:27 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

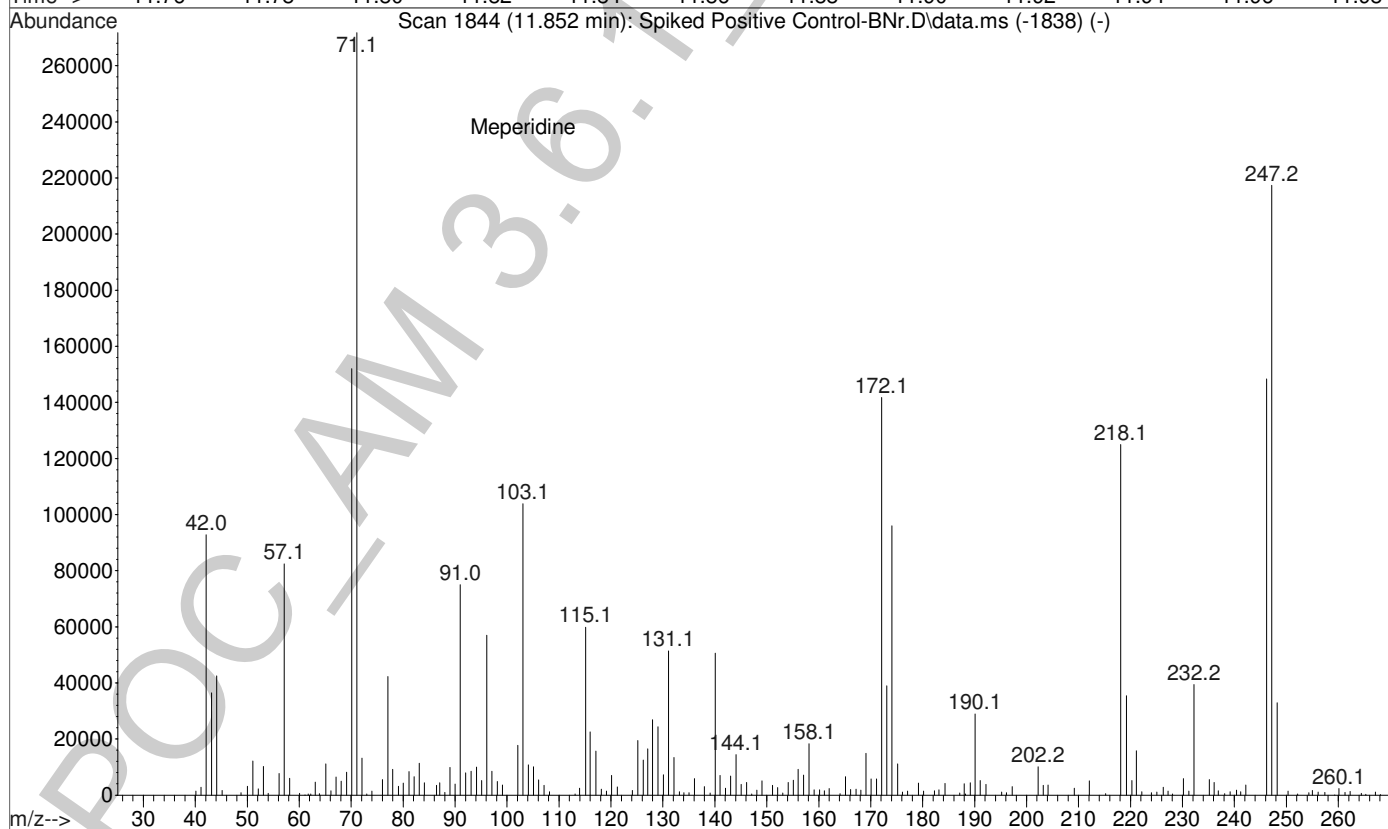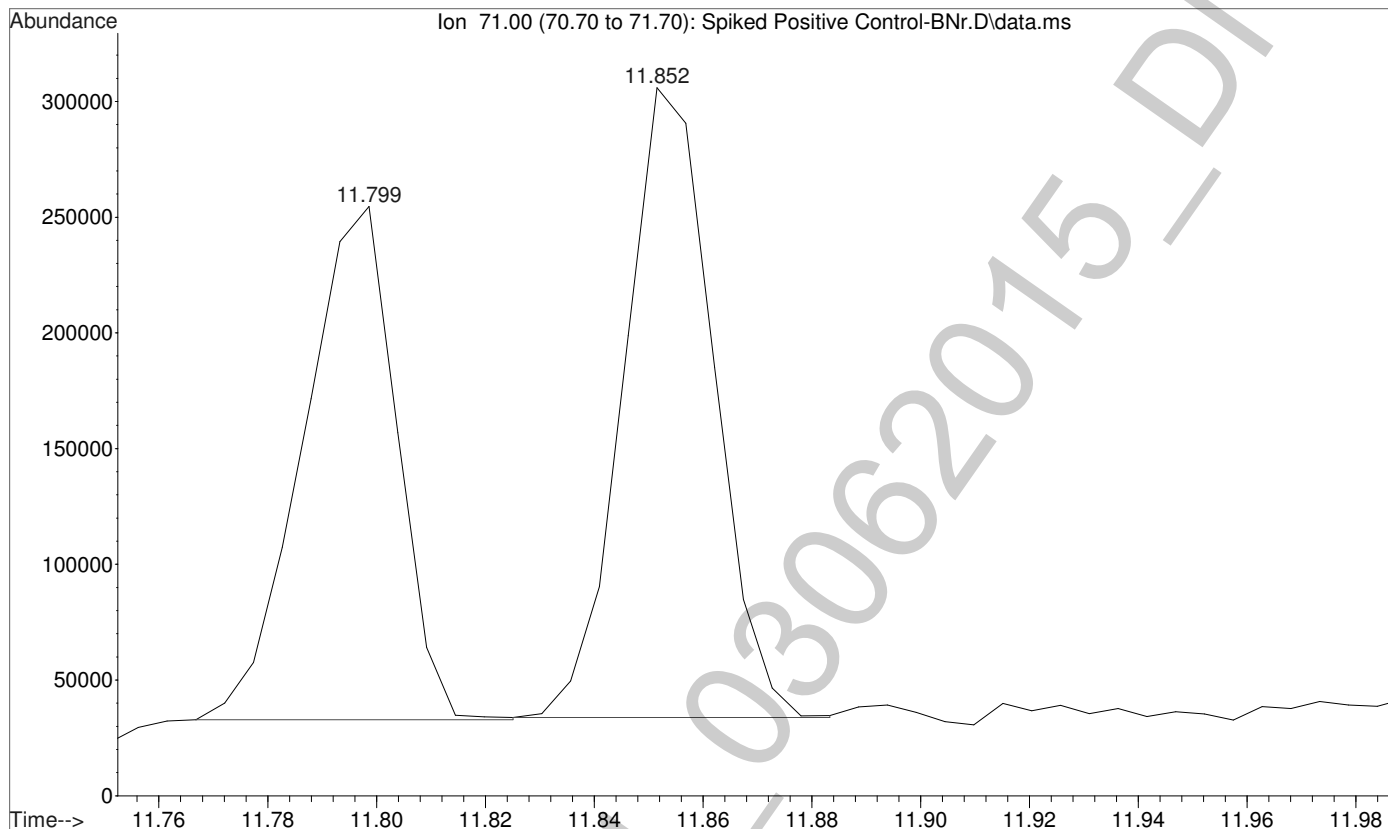



File :C:\gcms\1\data\Blood\030615BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 06 Mar 2015 11:27 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

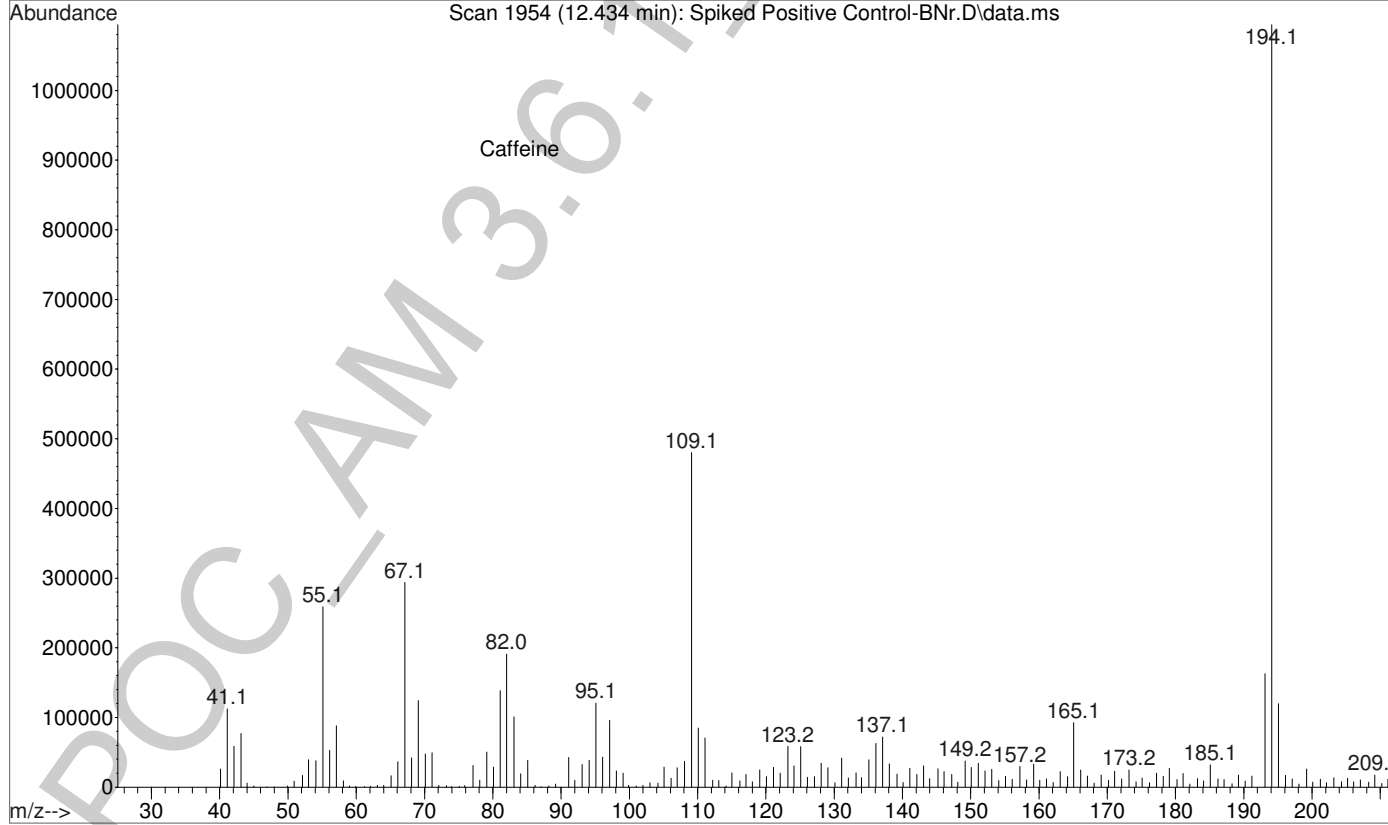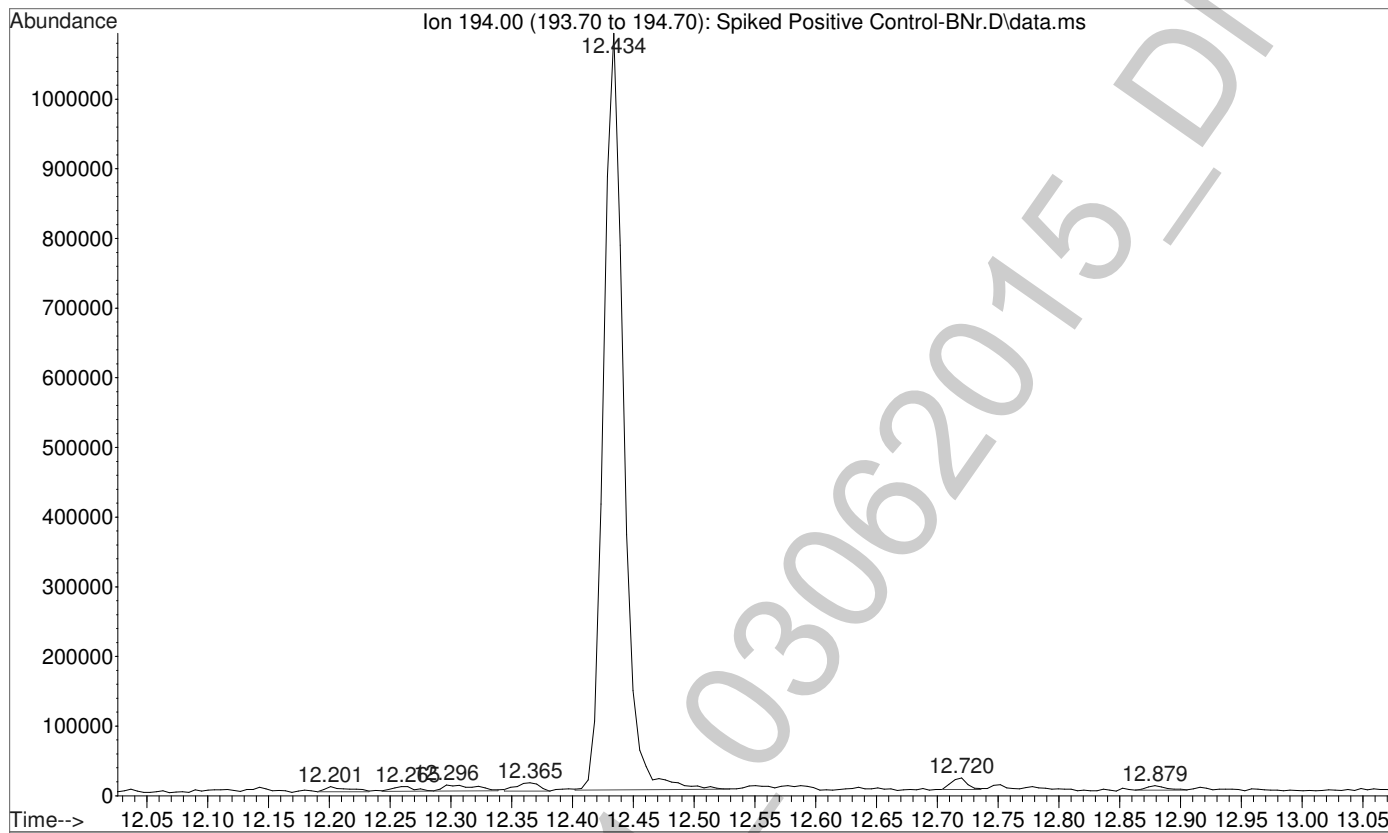



File :C:\gcms\1\data\Blood\030615BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 06 Mar 2015 11:27 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

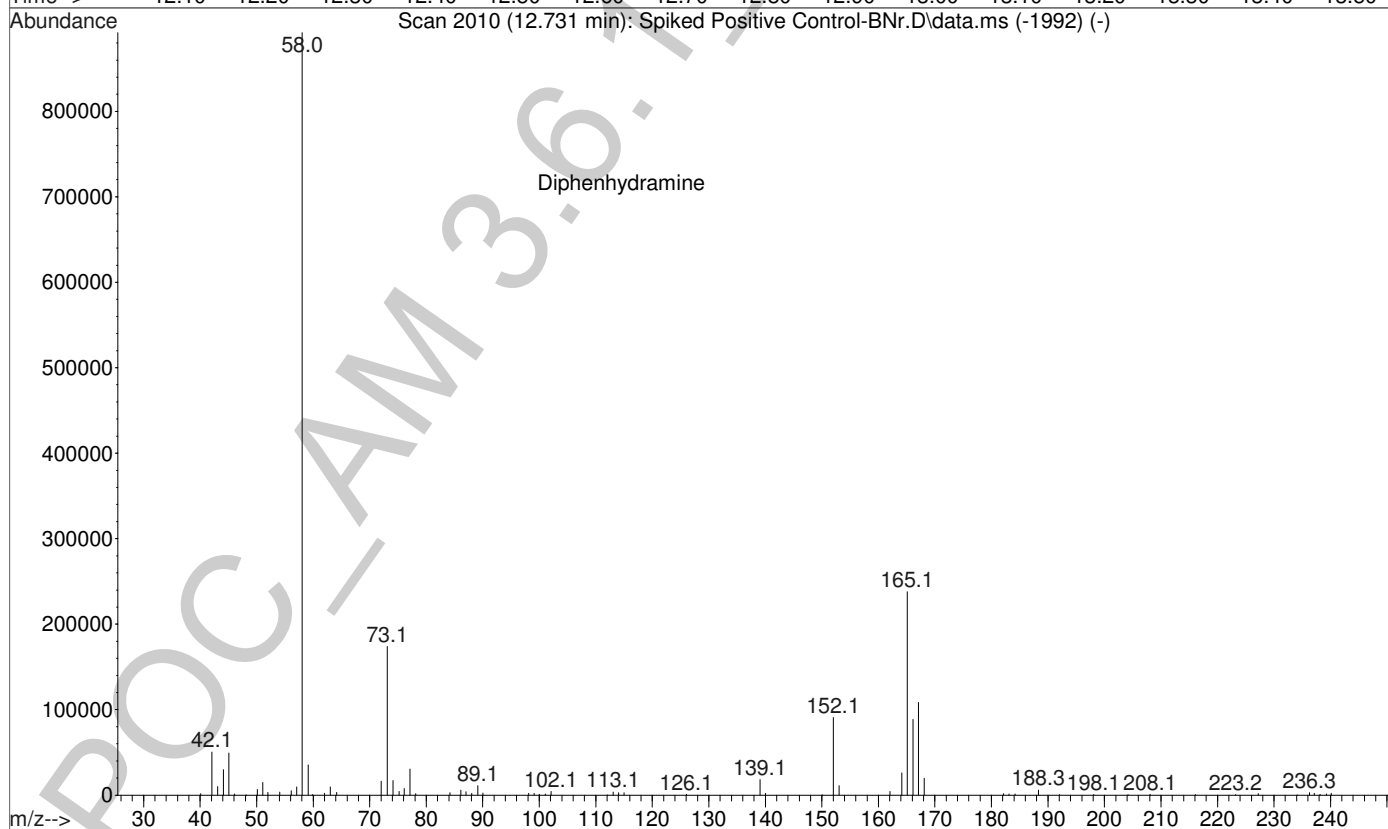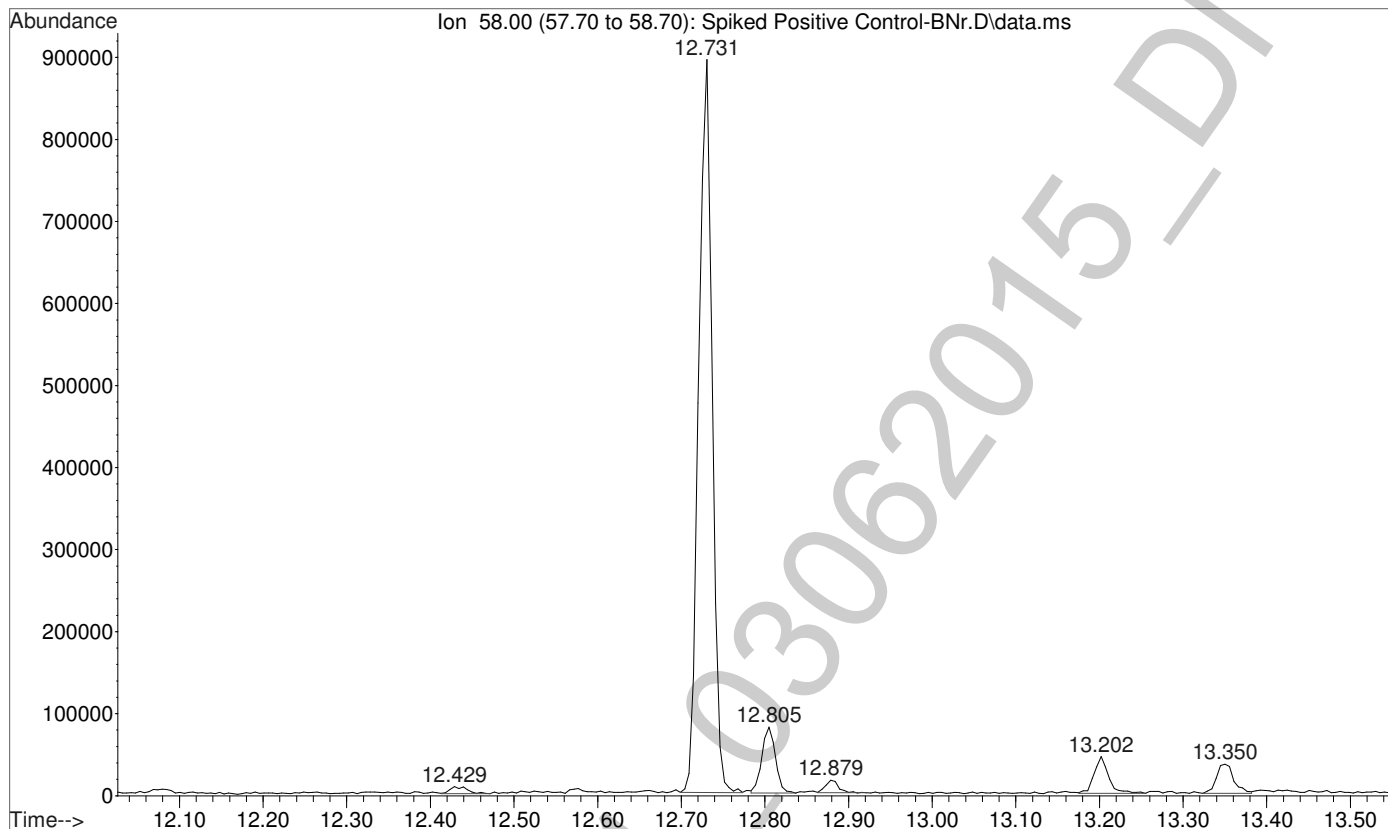



File :C:\gcms\1\data\Blood\030615BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 06 Mar 2015 11:27 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

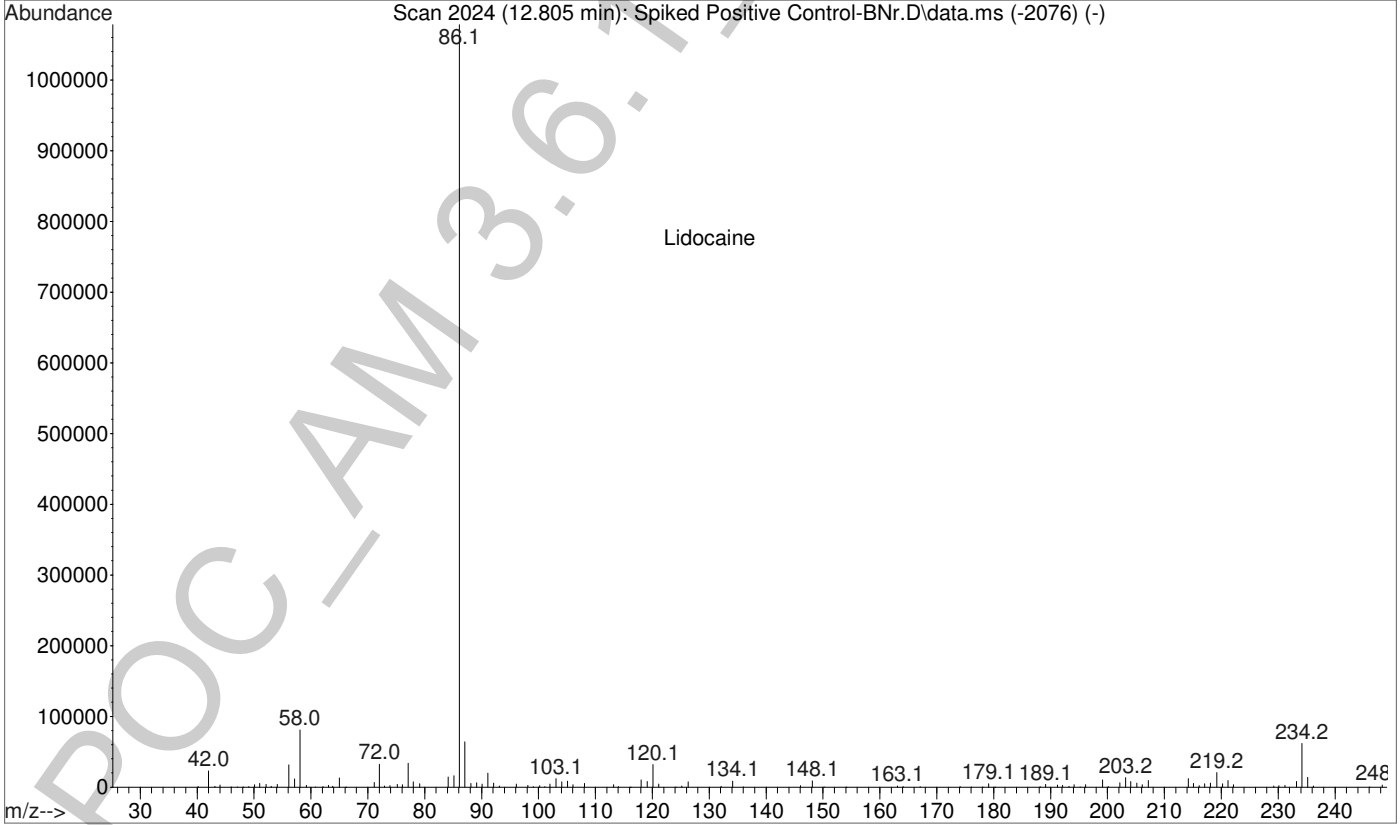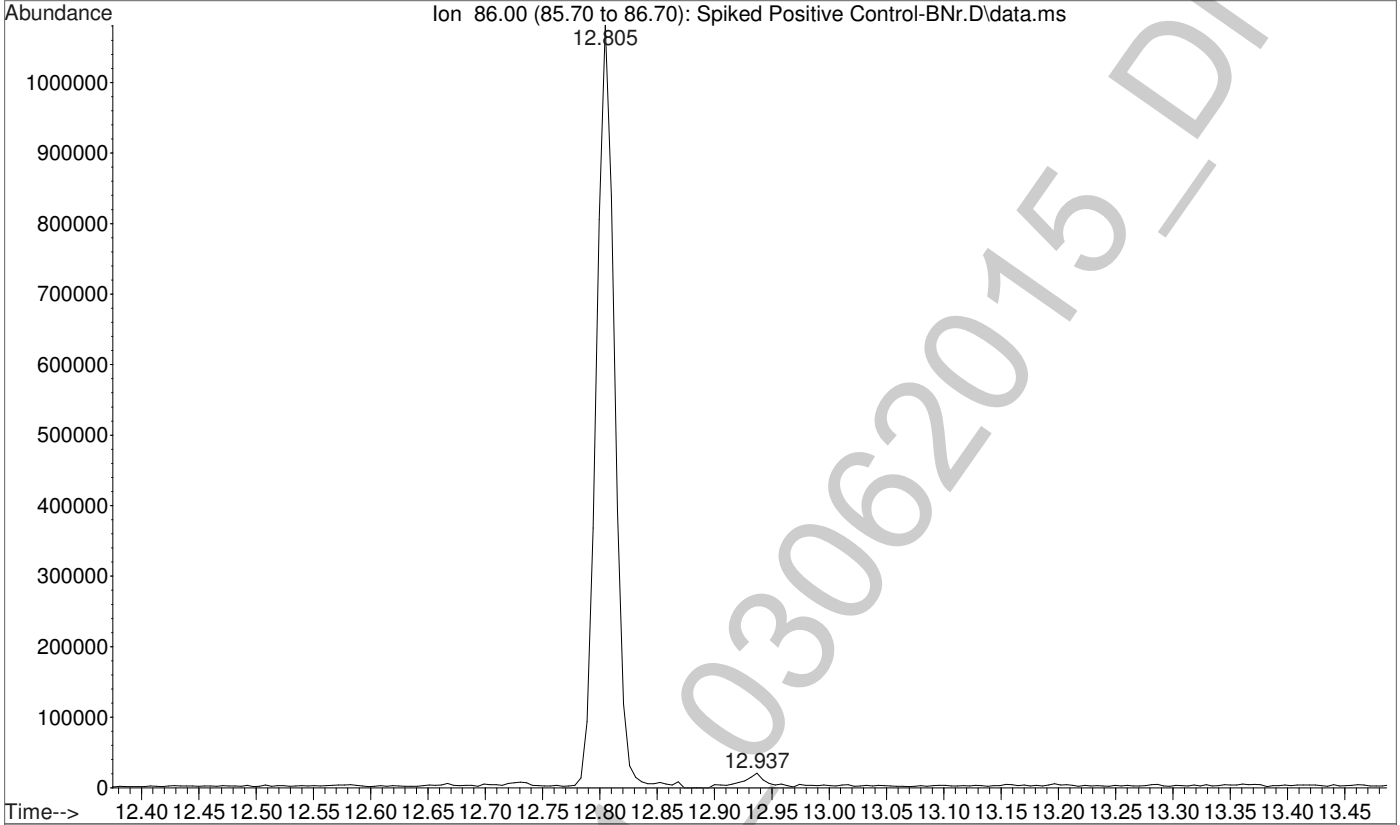



File :C:\gcms\1\data\Blood\030615BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 06 Mar 2015 11:27 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

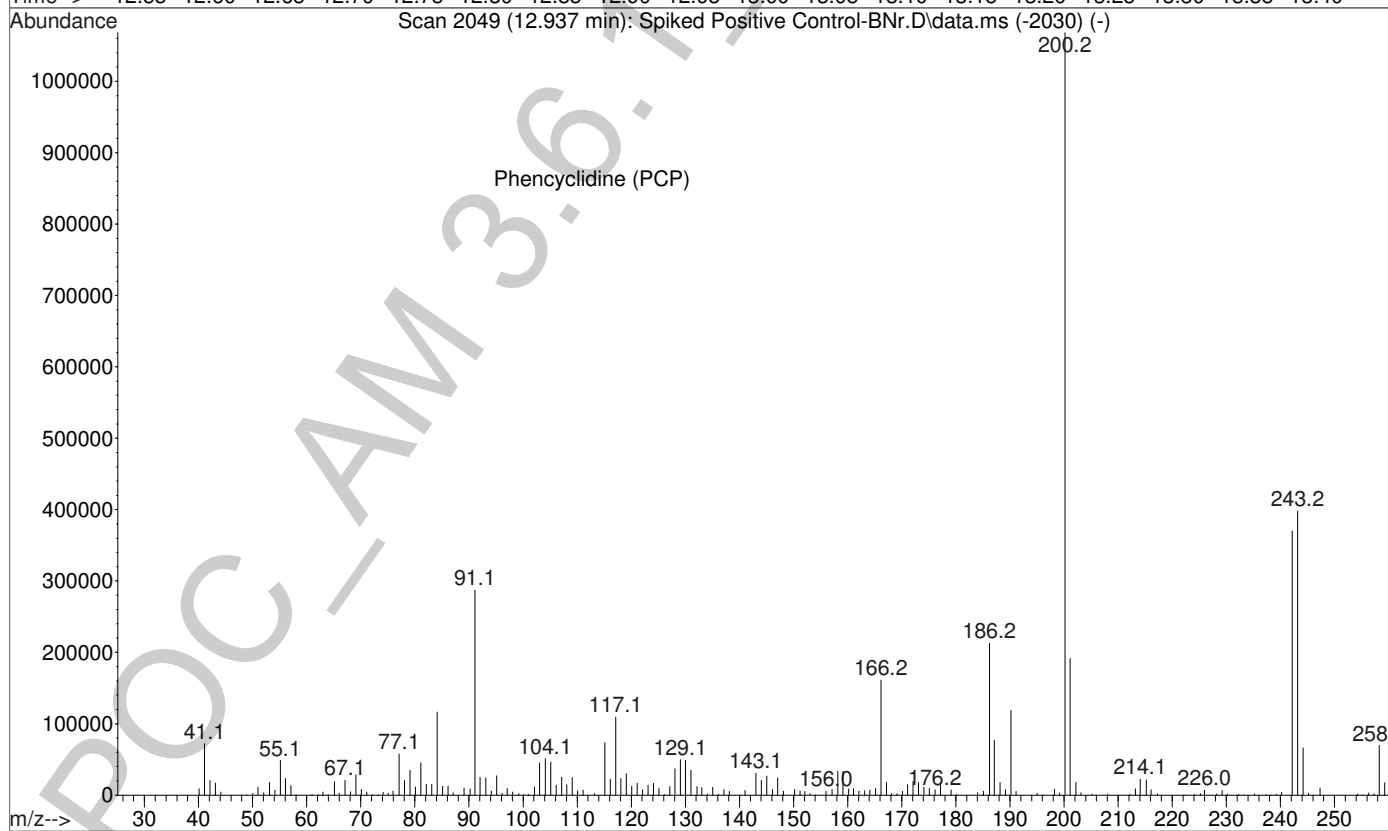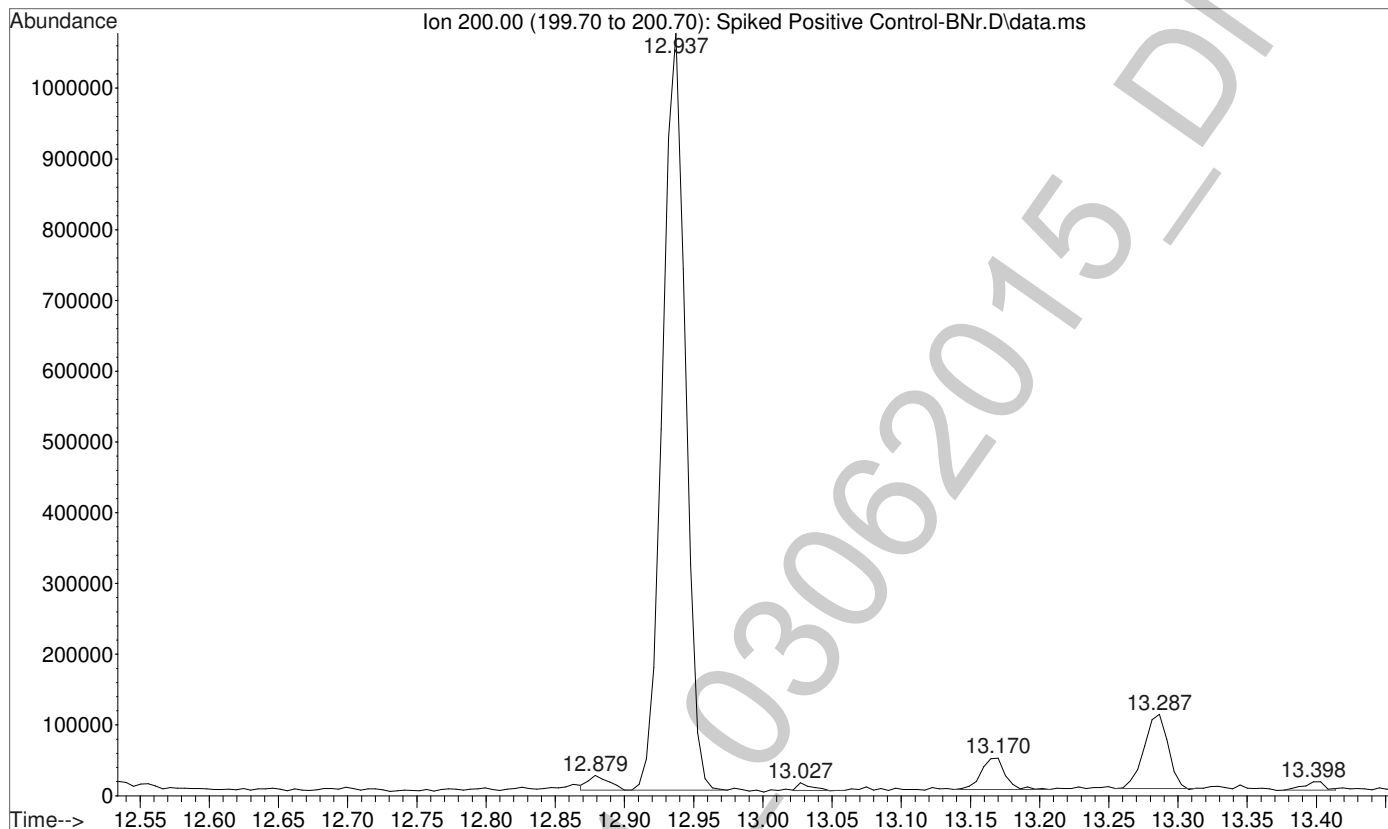



File :C:\gcms\1\data\Blood\030615BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 06 Mar 2015 11:27 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

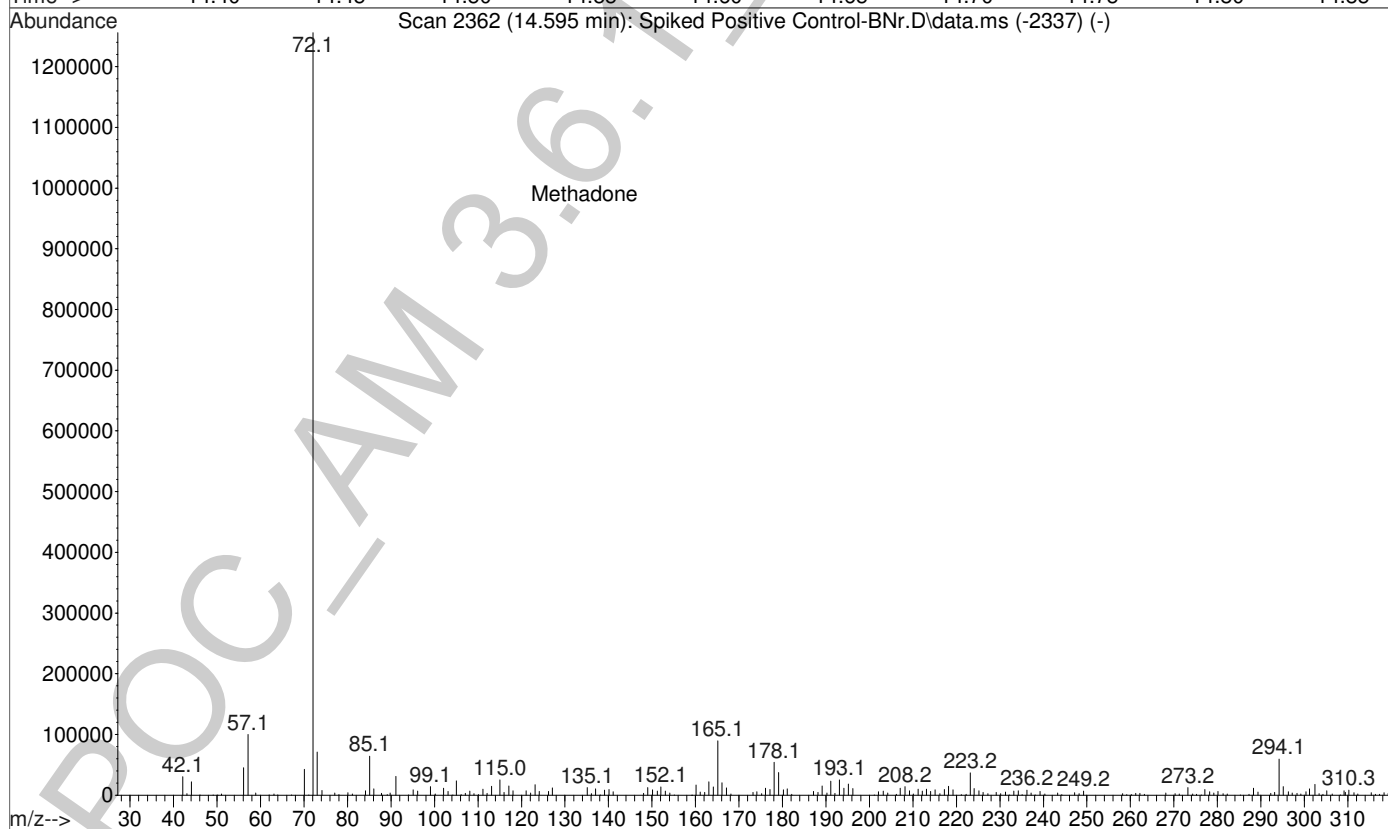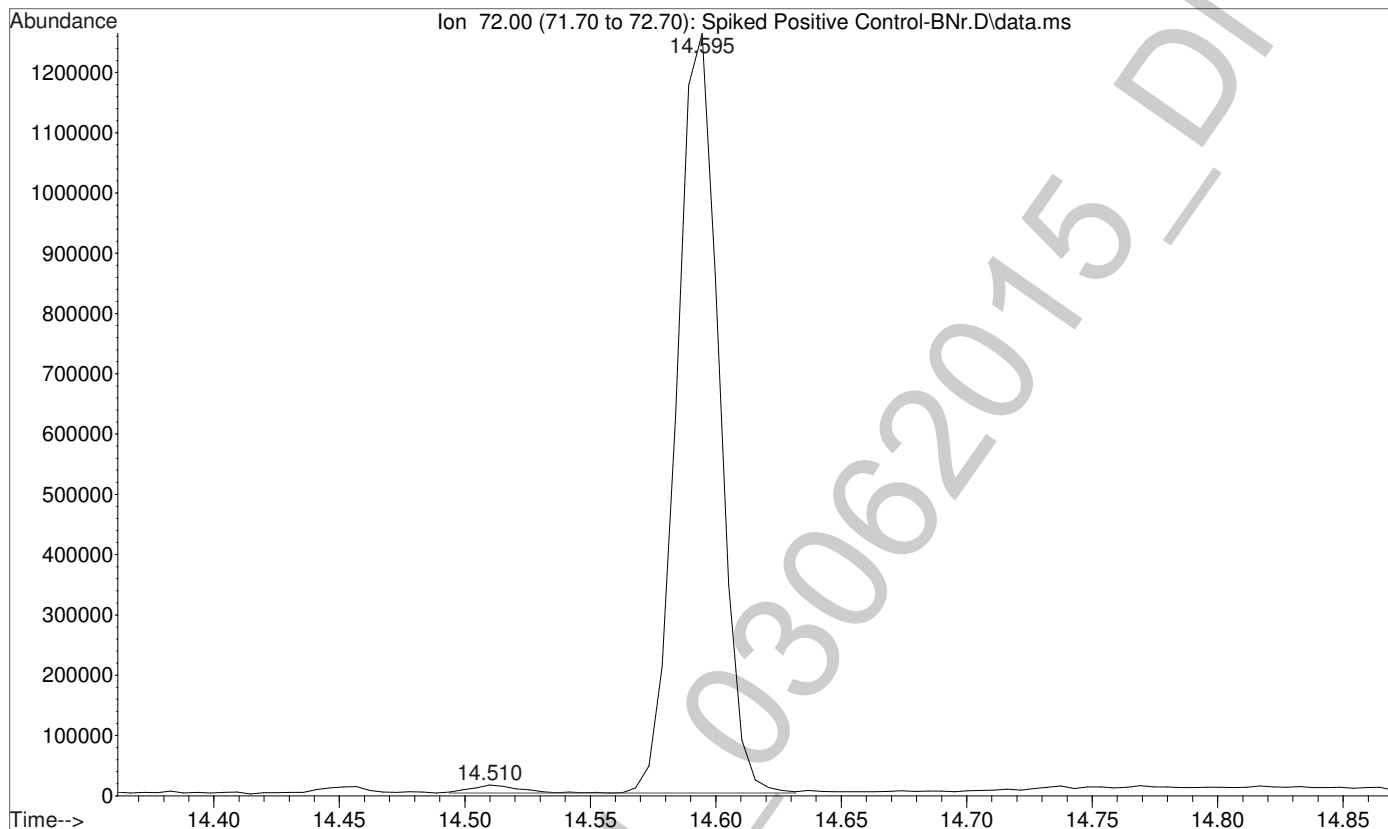



File :C:\gcms\1\data\Blood\030615BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 06 Mar 2015 11:27 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

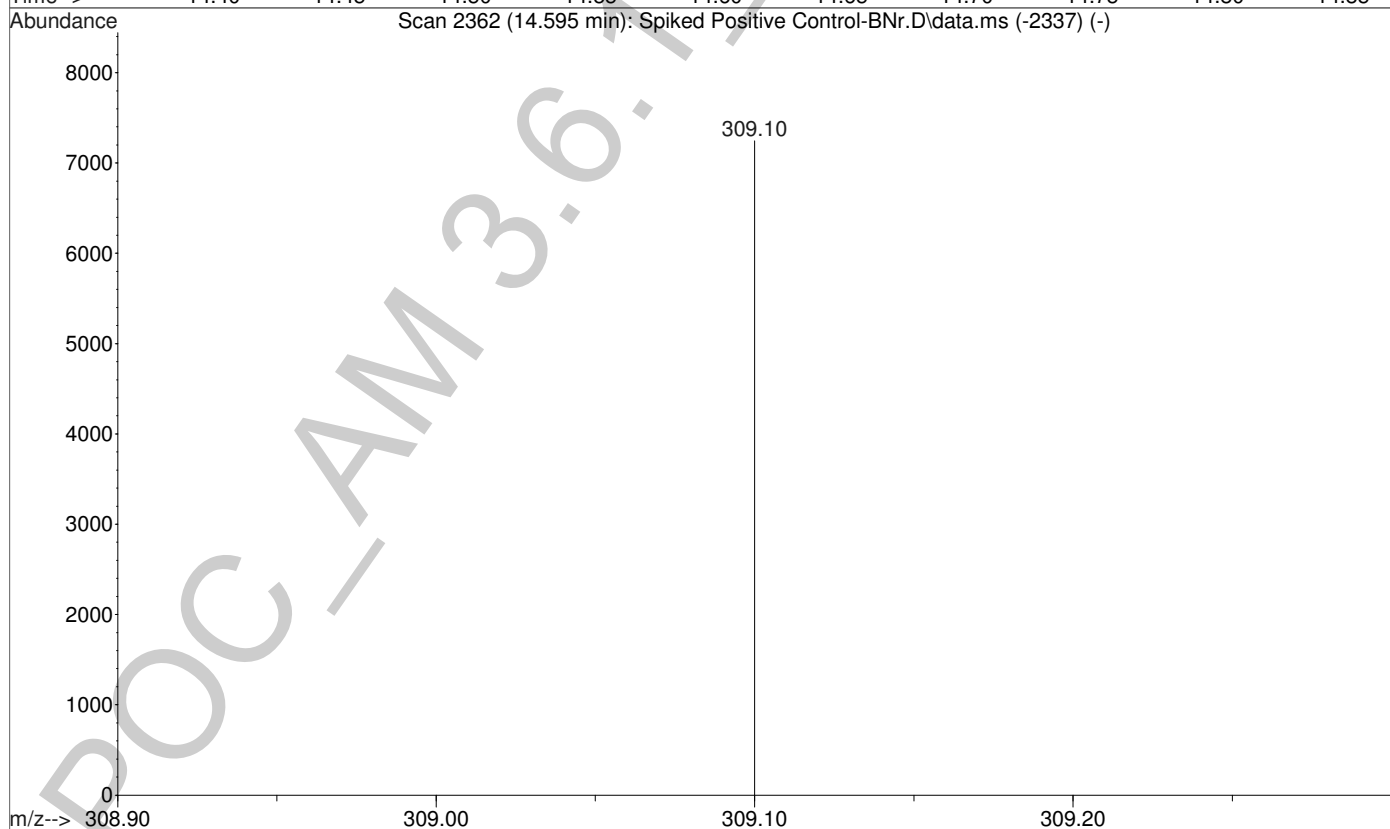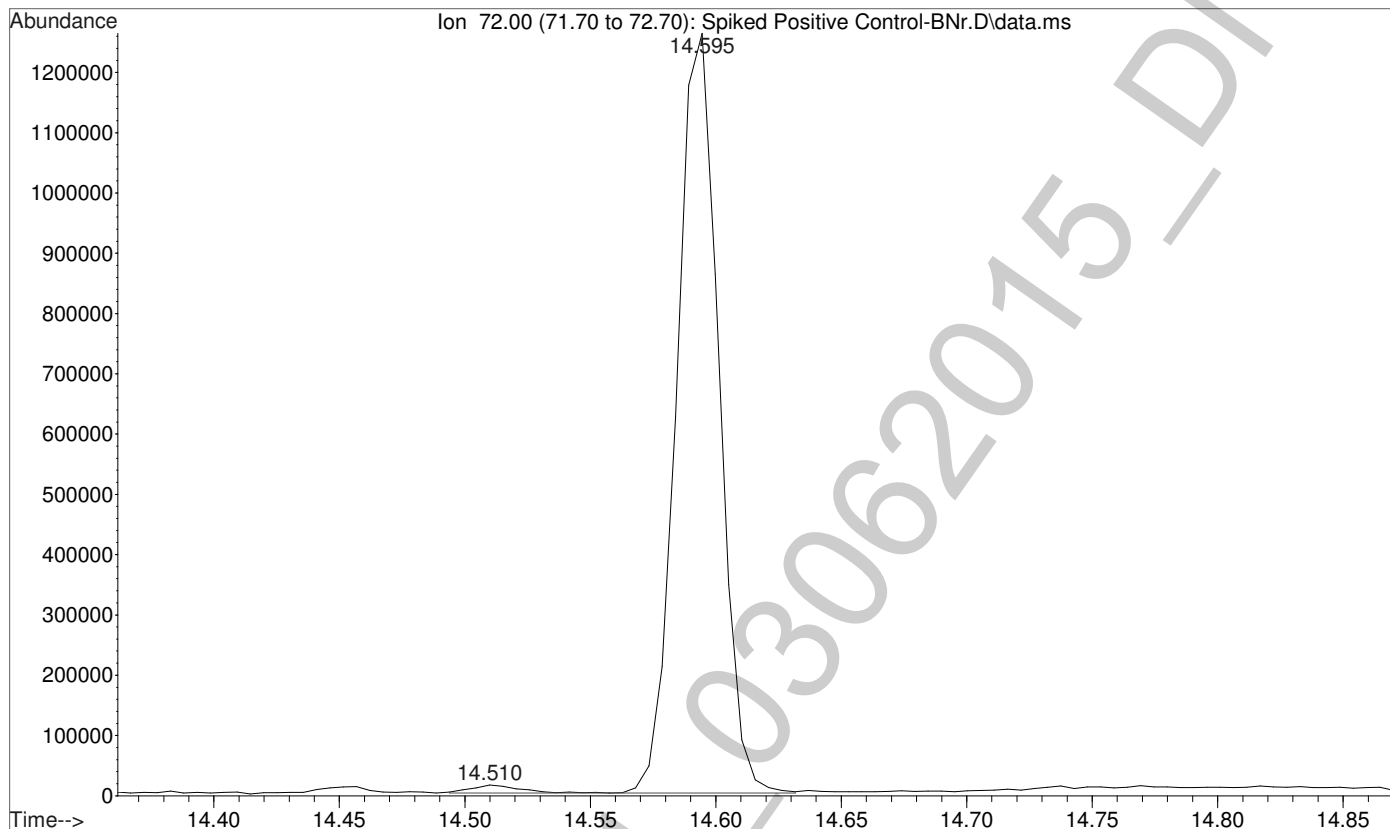



File :C:\gcms\1\data\Blood\030615BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 06 Mar 2015 11:27 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

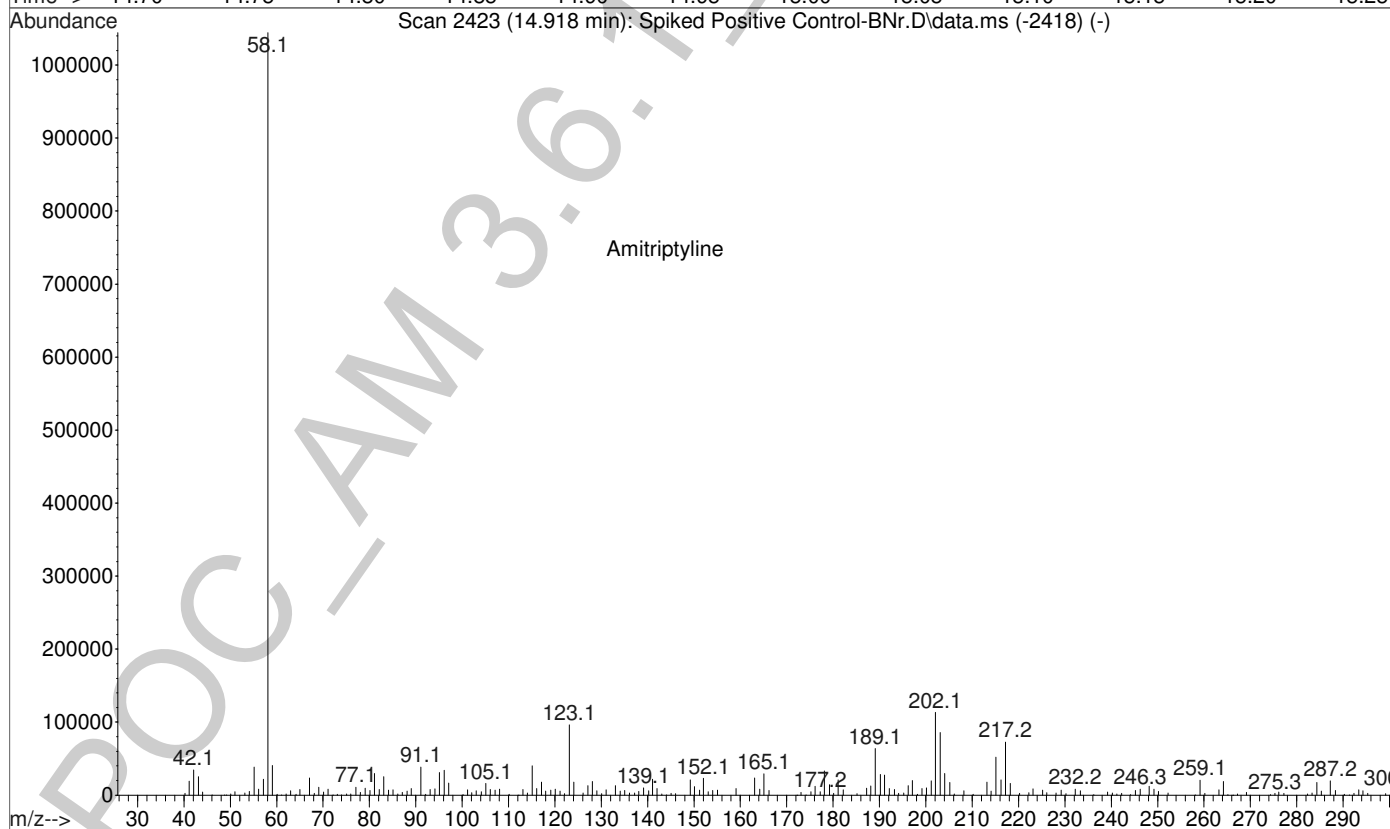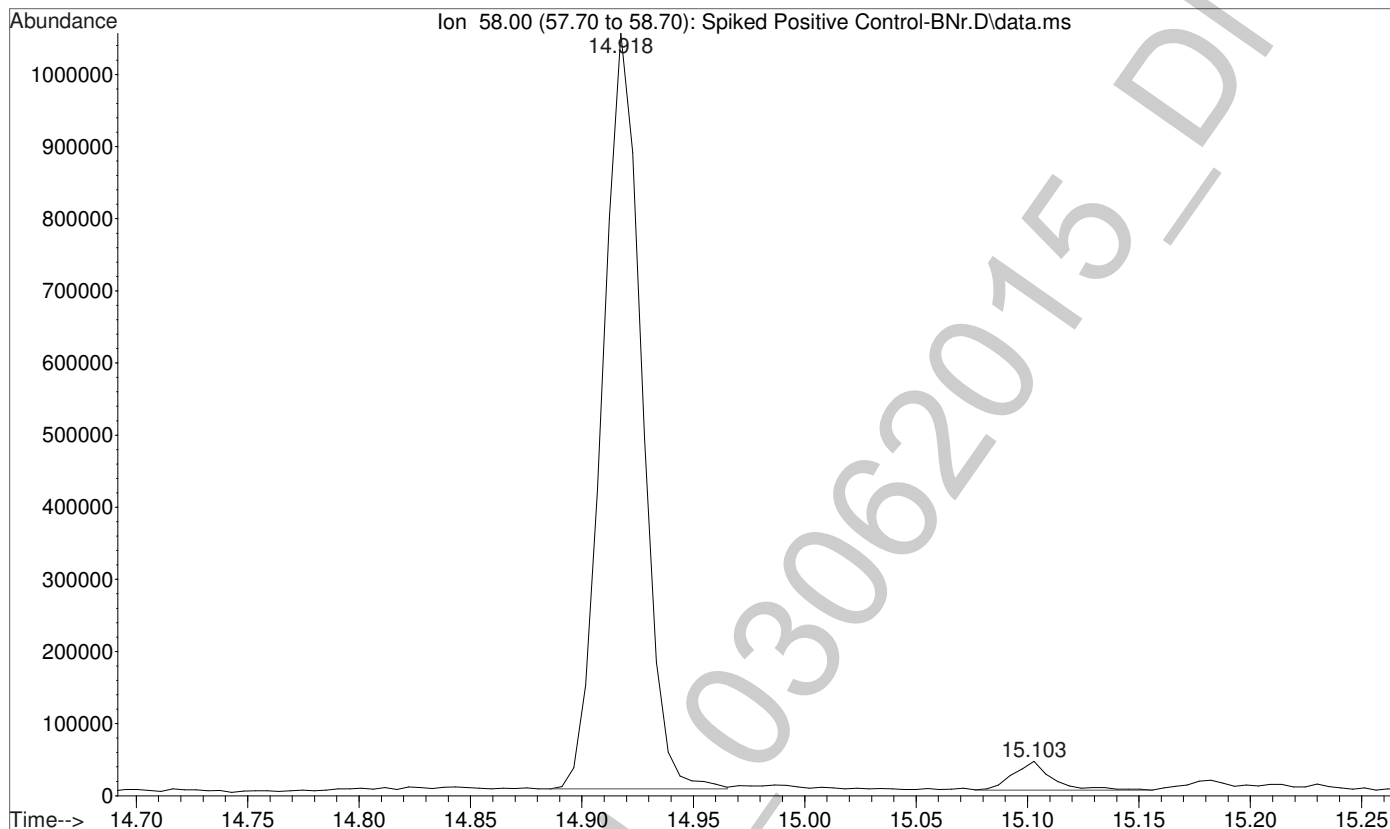



File :C:\gcms\1\data\Blood\030615BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 06 Mar 2015 11:27 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

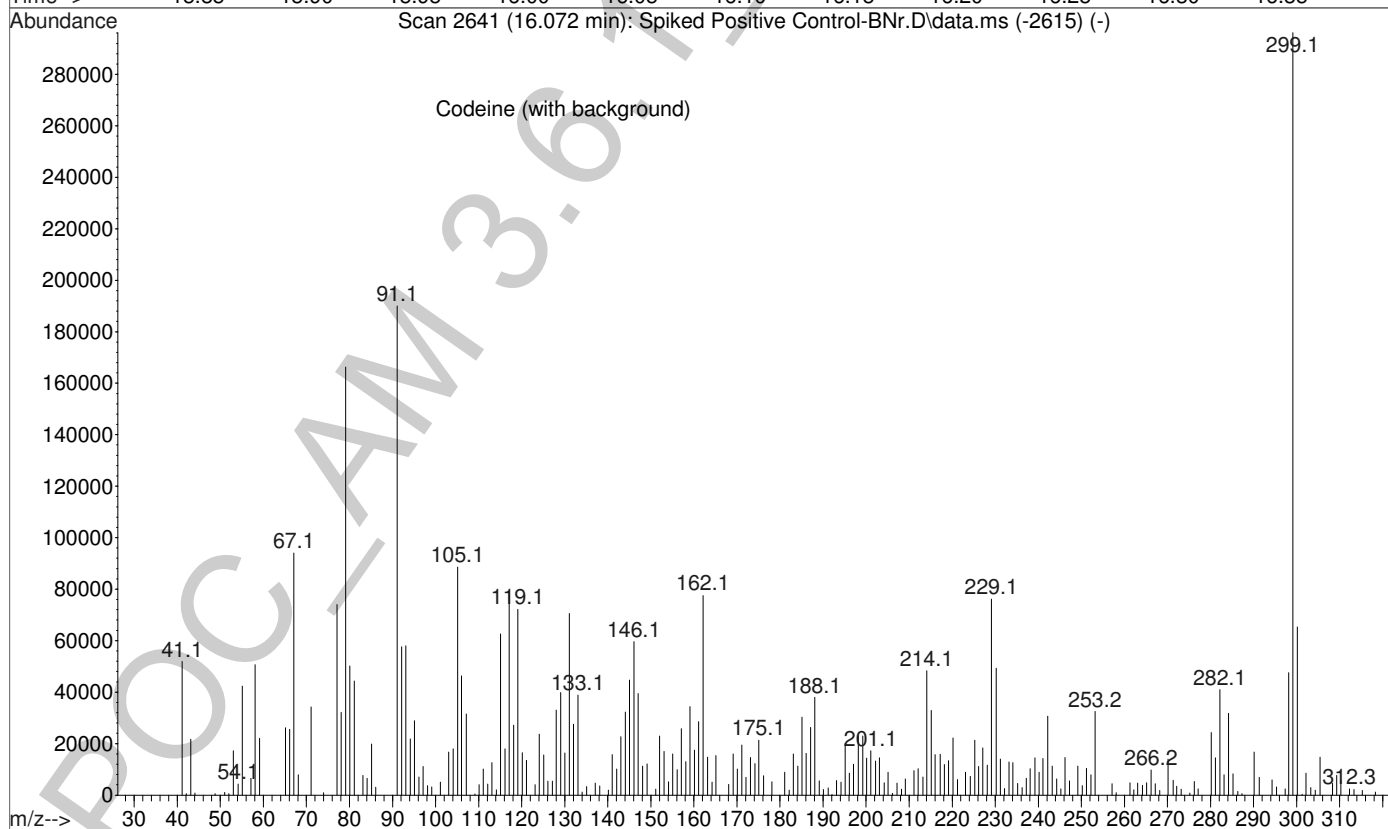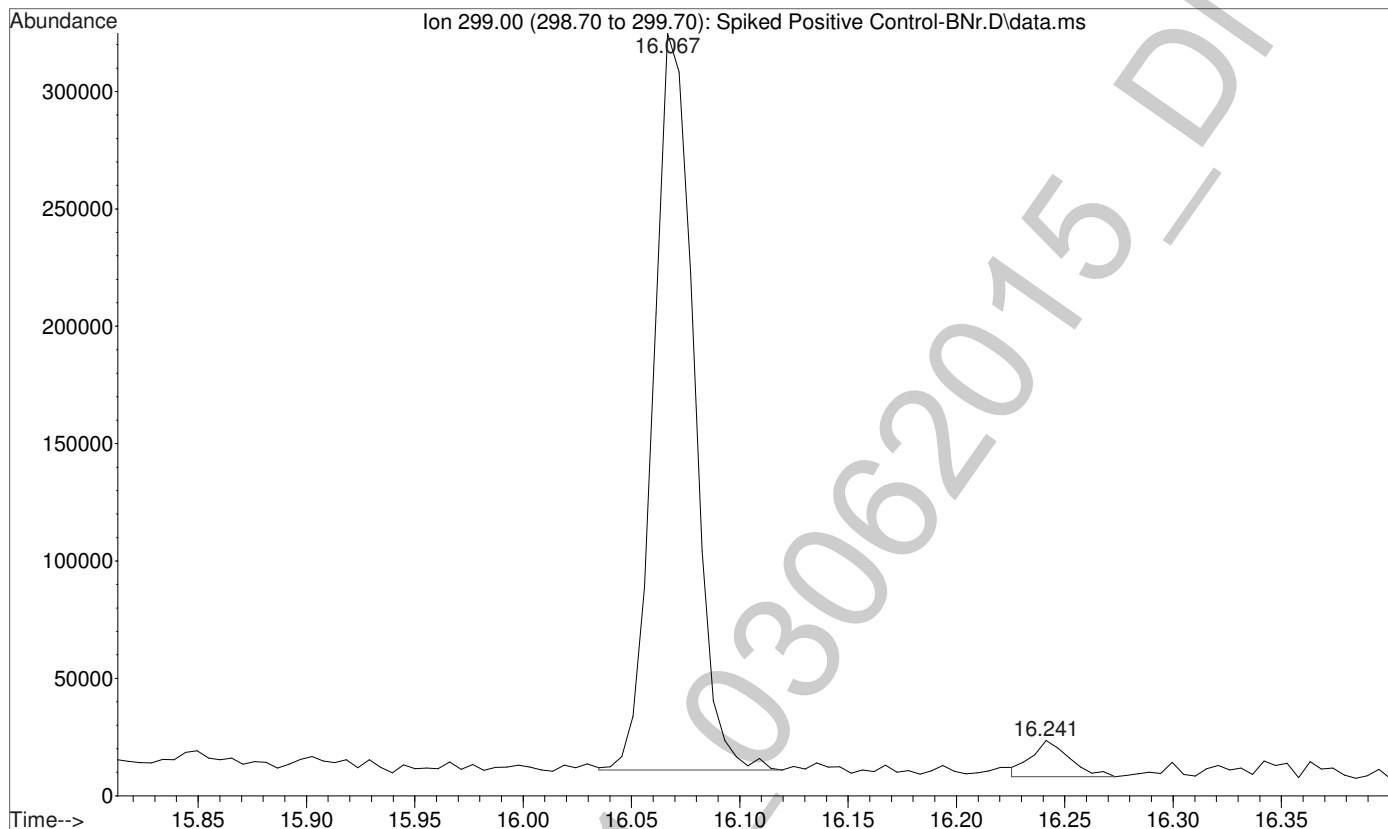



File :C:\gcms\1\data\Blood\030615BN\Reinjection Longer GC Method\S
... piked Positive Control-BNr.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 06 Mar 2015 11:27 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

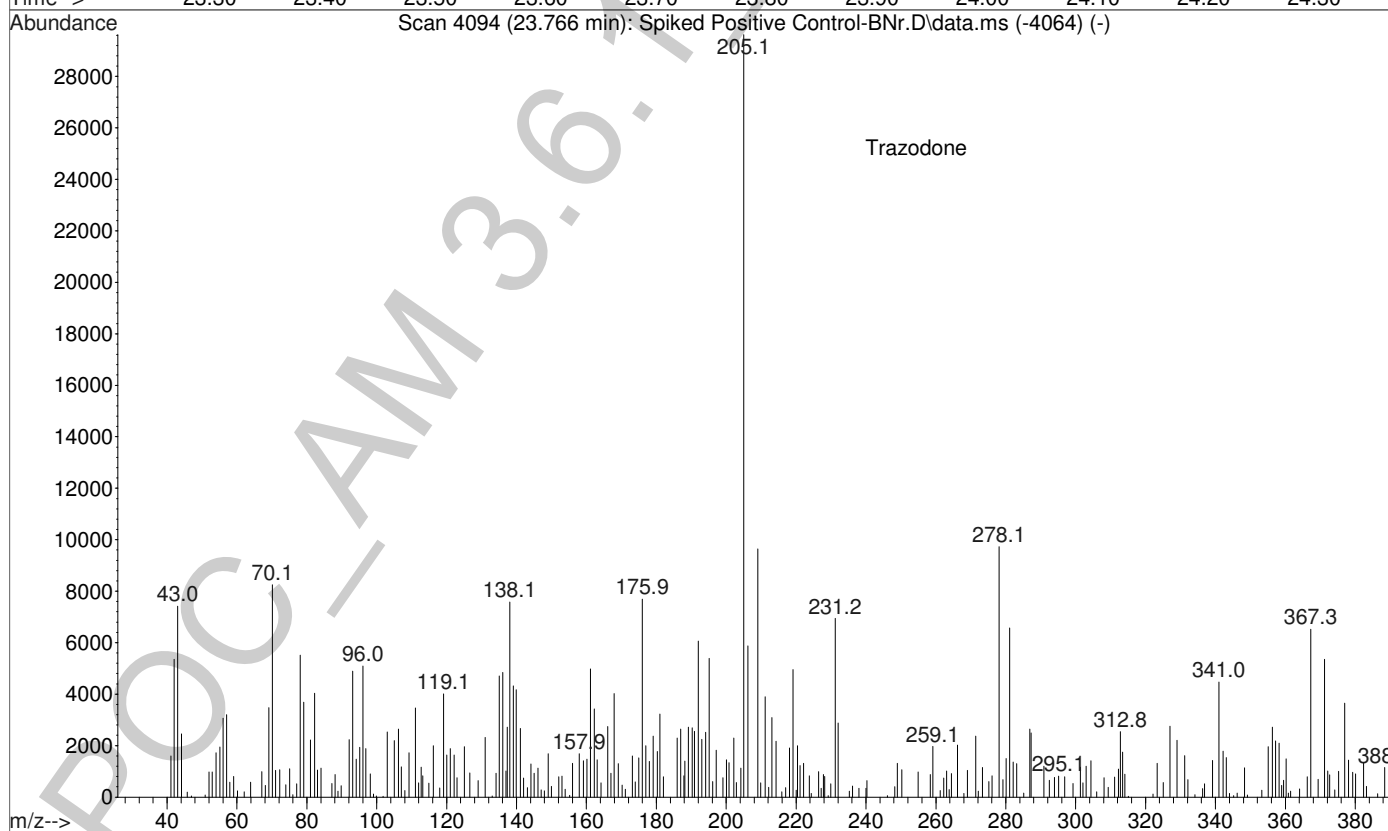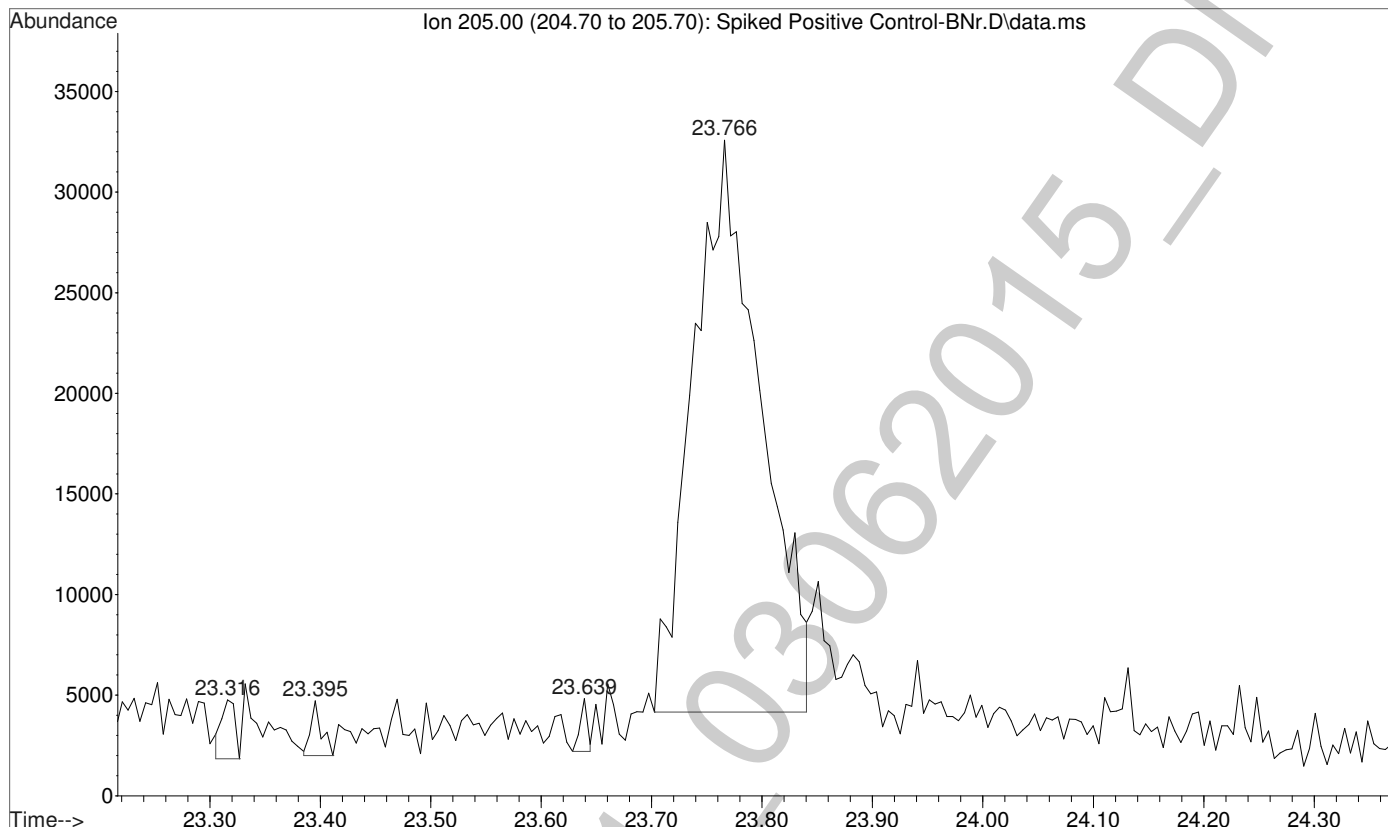

File :C:\gcms\1\data\Blood\030615BN\Reinjection Longer GC Method\p
... rbLK2r.D
Operator : 5LAB-C01\ISPuser
Instrument : Major Mass Spec
Acquired : 06 Mar 2015 12:01 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Solvent Blank
Misc Info : Chloroform

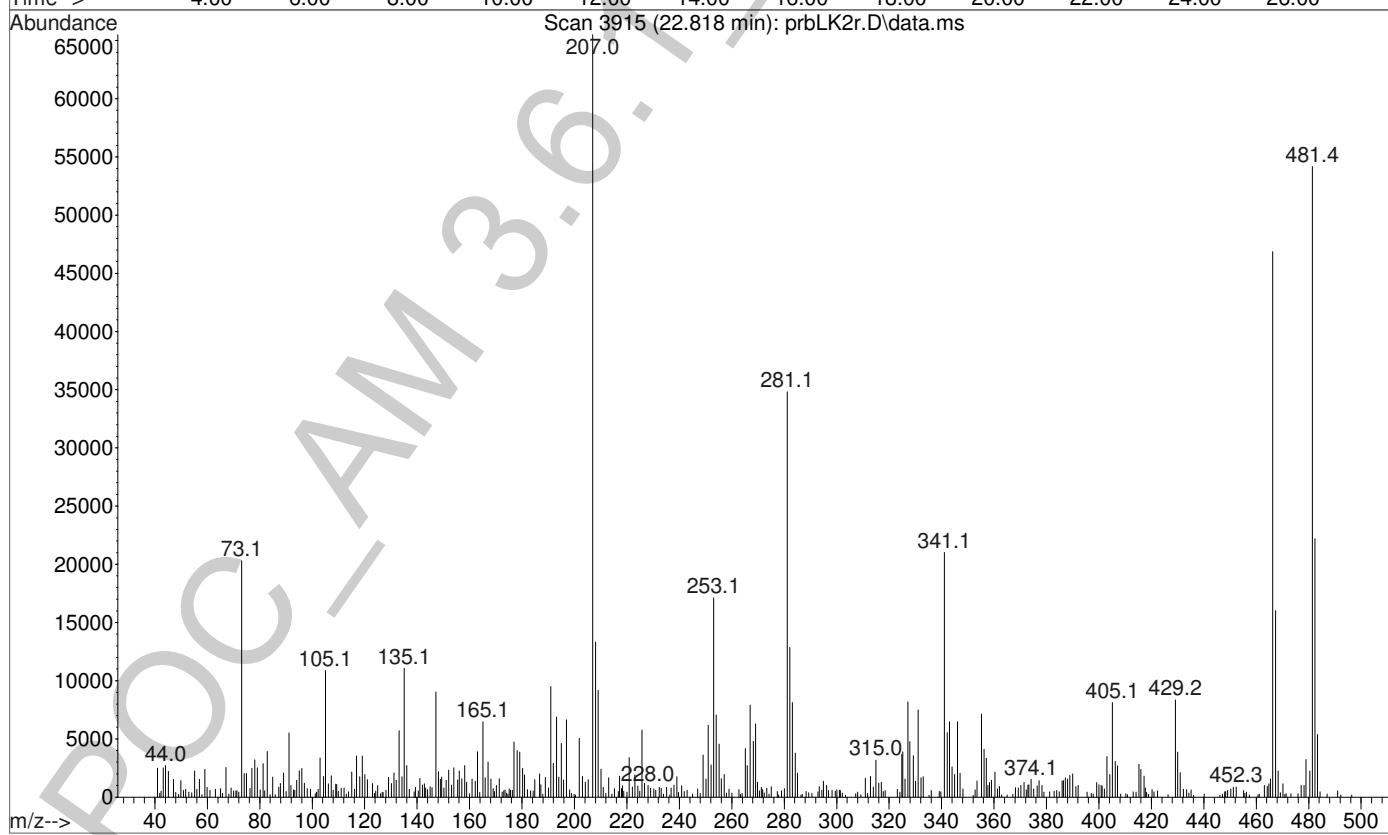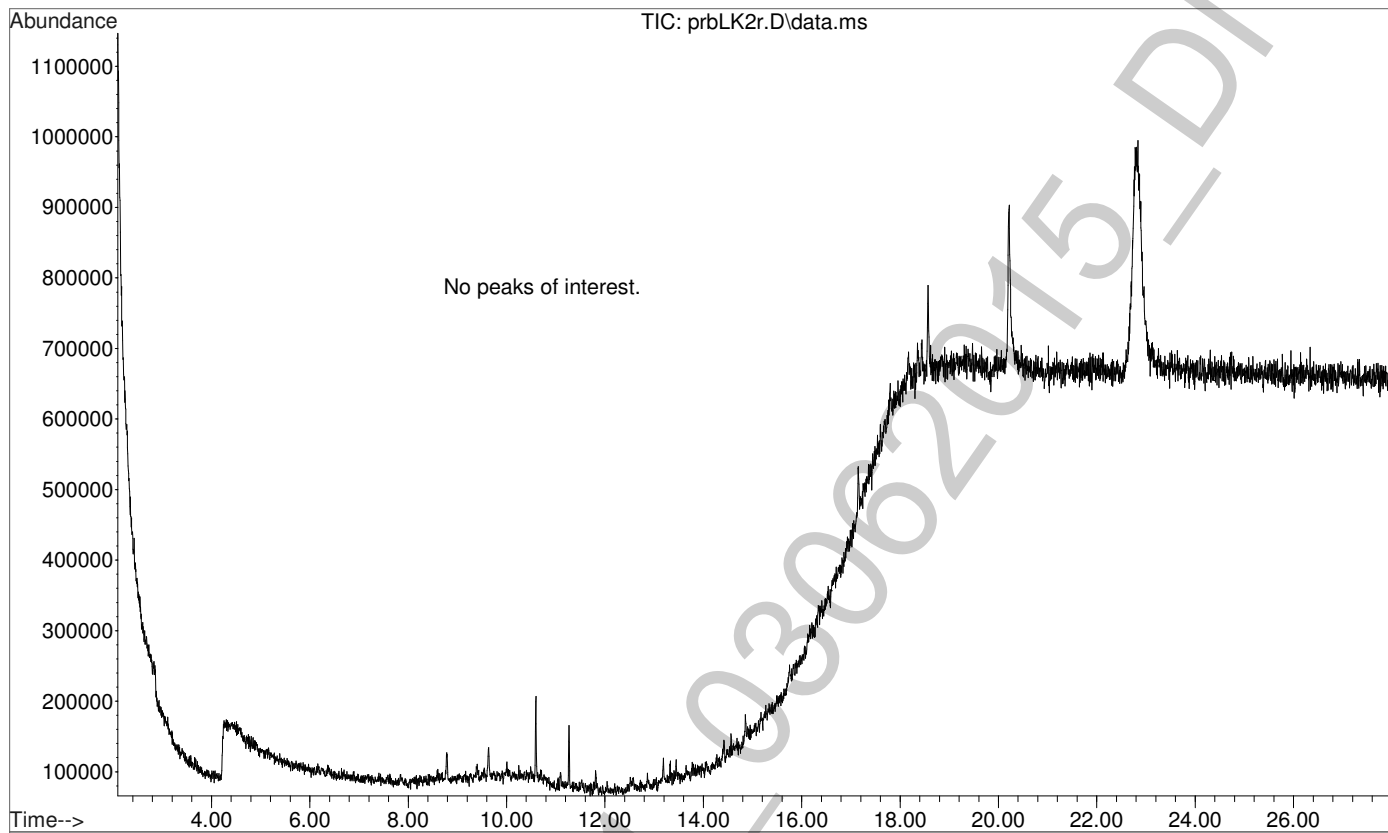

File :C:\gcms\1\data\Blood\030615BN\POSTBLK.D
Operator : 5LAB-C01\ISPuser
Acquired : 09 Mar 2015 00:56 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: BLK
Misc Info : Chloroform
Vial Number: 73

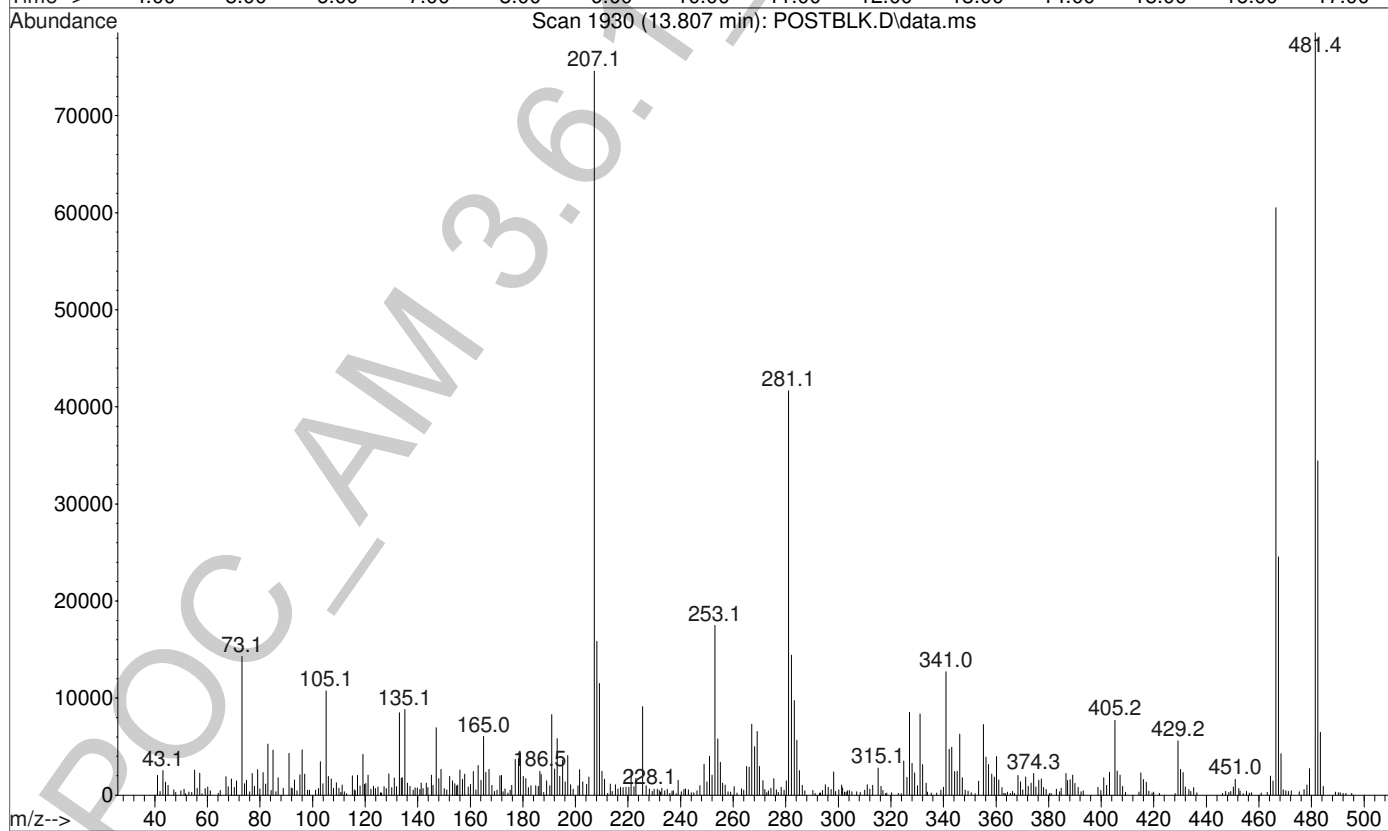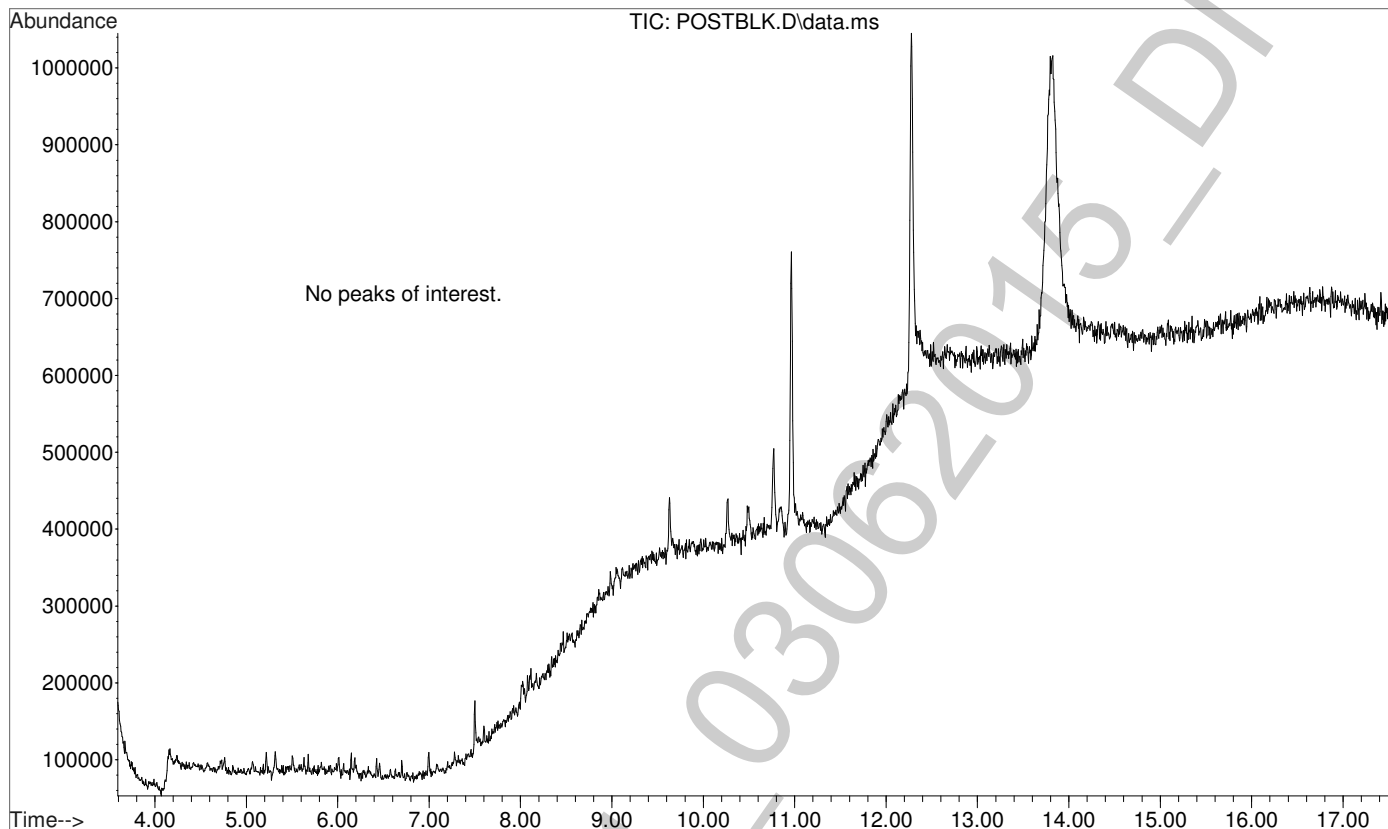

File :C:\gcms\1\data\Blood\030615BN\AFTER.D
Operator : 5LAB-C01\ISPuser
Acquired : 09 Mar 2015 01:18 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: BLK
Misc Info : Chloroform
Vial Number: 72

