

























Worklist: 858

reviewed 11-4-15 by BAW


Byyle

10/3/2015



<u>LAB_CASE</u>	<u>ITEM</u>	<u>TASK_ID</u>	<u>DESCRIPTION</u>	
C2015-1351	1	42408	3.6.1 Blood base neutral confirr	
C2015-1516	1	39889	3.6.1 Blood base neutral confirr	
C2015-1523	1	39990	3.6.1 Blood base neutral confirr	
C2015-1552	1	40160	3.6.1 Blood base neutral confirr	
C2015-1607	1	40860	3.6.1 Blood base neutral confirr	
M2015-3147	1	42906	3.6.1 Blood base neutral confirr	
M2015-3207	1	40857	3.6.1 Blood base neutral confirr	
M2015-3227	1	40939	3.6.1 Blood base neutral confirr	
M2015-3237	2	41262	3.6.1 Blood base neutral confirr	
M2015-3267	1	41225	3.6.1 Blood base neutral confirr	
M2015-3274	1	41278	3.6.1 Blood base neutral confirr	
M2015-3276	1	41292	3.6.1 Blood base neutral confirr	
M2015-3289	1	41341	3.6.1 Blood base neutral confirr	
M2015-3336	2	41831	3.6.1 Blood base neutral confirr	
M2015-3360	1	41608	3.6.1 Blood base neutral confirr	
M2015-3361	1	41611	3.6.1 Blood base neutral confirr	
M2015-3377	1	41686	3.6.1 Blood base neutral confirr	
M2015-3402	2	42128	3.6.1 Blood base neutral confirr	
M2015-3424	3	42350	3.6.1 Blood base neutral confirr	
P2015-2011	1	41145	3.6.1 Blood base neutral confirr	
P2015-2017	1	41219	3.6.1 Blood base neutral confirr	
P2015-2018	1	41222	3.6.1 Blood base neutral confirr	
P2015-2025	1	41259	3.6.1 Blood base neutral confirr	

Worklist: 858



<u>LAB CASE</u>	<u>ITEM</u>	<u>TASK ID</u>	<u>DESCRIPTION</u>	
P2015-2033	1	41370	3.6.1 Blood base neutral confirr	
P2015-2034	1	41373	3.6.1 Blood base neutral confirr	
P2015-2068	1	41549	3.6.1 Blood base neutral confirr	
P2015-2083	1	41670	3.6.1 Blood base neutral confirr	
P2015-2084	1	41674	3.6.1 Blood base neutral confirr	
P2015-2089	1	41732	3.6.1 Blood base neutral confirr	
P2015-2092	1	41746	3.6.1 Blood base neutral confirr	
P2015-2093	1	41749	3.6.1 Blood base neutral confirr	
P2015-2096	1	41797	3.6.1 Blood base neutral confirr	
P2015-2097	1	41800	3.6.1 Blood base neutral confirr	
P2015-2113	1	41997	3.6.1 Blood base neutral confirr	
P2015-2123	1	42125	3.6.1 Blood base neutral confirr	
P2015-2129	1	42164	3.6.1 Blood base neutral confirr	
P2015-2161	1	42343	3.6.1 Blood base neutral confirr	
P2015-2162	1	42353	3.6.1 Blood base neutral confirr	
P2015-2184	1	42501	3.6.1 Blood base neutral confirr	
P2015-2186	1	42508	3.6.1 Blood base neutral confirr	
P2015-2194	1	42729	3.6.1 Blood base neutral confirr	

Verified that all ALS vials were in the correct rack positions on 10/02/2015. 



simulate_sequence.log
Simulate Run Sequence Fri Oct 02 22:56:14 2015

Instrument Name: Major Mass Spec
Sequence File: C:\Users\ISPuser\Desktop\Sequences\DD-BNSB100215.sequence.xml
Comment: MassHunter sequence
Operator: ISP\datastor
Data Path: D:\DATA\DND\2015\100215\
Method Path: D:\MassHunter\GCMS\1\methods\

Line	Type	Vials	DataFile	Sample Name
Acquisition Method: BNSB120510.M				
1)	Sample	100	Prerun Solvent Blank	Pre-run Solvent Blank
2)	Sample	1	Negative Control-BN	Negative Control -
...0689	3)	Sample	2	Spiked Positive Control-BN Positive Control
4)	Sample	99	prBLK2	solvent Blank
Acquisition Method: GBT092509-Delta EMV.M				
5)	Sample	100	Prerun Solvent Blankr	Pre-run Solvent Blank
6)	Sample	1	Negative Control-BNr	Negative Control -
...0689	7)	Sample	2	Spiked Positive Control-BNr Positive Control
8)	Sample	99	prBLK2r	solvent Blank
Acquisition Method: BNSB120510.M				
9)	Sample	98	C2015-1351-1-BNBLK	Lab No.: C2015-1351-1
10)	Sample	3	C2015-1351-1-BN	Lab No.: C2015-1351-1
11)	Sample	97	C2015-1516-1-BNBLK	Lab No.: C2015-1516-1
12)	Sample	4	C2015-1516-1-BN	Lab No.: C2015-1516-1
13)	Sample	96	C2015-1523-1-BNBLK	Lab No.: C2015-1523-1
14)	Sample	5	C2015-1523-1-BN	Lab No.: C2015-1523-1
15)	Sample	95	C2015-1552-1-BNBLK	Lab No.: C2015-1552-1
16)	Sample	6	C2015-1552-1-BN	Lab No.: C2015-1552-1
17)	Sample	94	C2015-1607-1-BNBLK	Lab No.: C2015-1607-1
18)	Sample	7	C2015-1607-1-BN	Lab No.: C2015-1607-1
19)	Sample	93	M2015-3147-1-BNBLK	Lab No.: M2015-3147-1
20)	Sample	8	M2015-3147-1-BN	Lab No.: M2015-3147-1
21)	Sample	92	M2015-3207-1-BNBLK	Lab No.: M2015-3207-1
22)	Sample	9	M2015-3207-1-BN	Lab No.: M2015-3207-1
23)	Sample	91	M2015-3227-1-BNBLK	Lab No.: M2015-3227-1
24)	Sample	10	M2015-3227-1-BN	Lab No.: M2015-3227-1
Acquisition Method: GBT092509-Delta EMV.M				
25)	Sample	98	C2015-1351-1-BNBLKr	Lab No.: C2015-1351-1
26)	Sample	3	C2015-1351-1-BNr	Lab No.: C2015-1351-1
27)	Sample	97	C2015-1516-1-BNBLKr	Lab No.: C2015-1516-1
28)	Sample	4	C2015-1516-1-BNr	Lab No.: C2015-1516-1
29)	Sample	96	C2015-1523-1-BNBLKr	Lab No.: C2015-1523-1
30)	Sample	5	C2015-1523-1-BNr	Lab No.: C2015-1523-1
31)	Sample	95	C2015-1552-1-BNBLKr	Lab No.: C2015-1552-1
32)	Sample	6	C2015-1552-1-BNr	Lab No.: C2015-1552-1
33)	Sample	94	C2015-1607-1-BNBLKr	Lab No.: C2015-1607-1
34)	Sample	7	C2015-1607-1-BNr	Lab No.: C2015-1607-1
35)	Sample	93	M2015-3147-1-BNBLKr	Lab No.: M2015-3147-1
36)	Sample	8	M2015-3147-1-BNr	Lab No.: M2015-3147-1
37)	Sample	92	M2015-3207-1-BNBLKr	Lab No.: M2015-3207-1
38)	Sample	9	M2015-3207-1-BNr	Lab No.: M2015-3207-1
39)	Sample	91	M2015-3227-1-BNBLKr	Lab No.: M2015-3227-1
40)	Sample	10	M2015-3227-1-BNr	Lab No.: M2015-3227-1
Acquisition Method: BNSB120510.M				
41)	Sample	90	M2015-3237-2-BNBLK	Lab No.: M2015-3237-2
42)	Sample	11	M2015-3237-2-BN	Lab No.: M2015-3237-2
43)	Sample	89	M2015-3267-1-BNBLK	Lab No.: M2015-3267-1
44)	Sample	12	M2015-3267-1-BN	Lab No.: M2015-3267-1



simulate_sequence.log			
45) Sample	88	M2015-3274-1-BNBLK	Lab No.: M2015-3274-1
46) Sample	13	M2015-3274-1-BN	Lab No.: M2015-3274-1
47) Sample	87	M2015-3276-1-BNBLK	Lab No.: M2015-3276-1
48) Sample	14	M2015-3276-1-BN	Lab No.: M2015-3276-1
49) Sample	86	M2015-3289-1-BNBLK	Lab No.: M2015-3289-1
50) Sample	15	M2015-3289-1-BN	Lab No.: M2015-3289-1
Acquisition Method: GBT092509-Delta EMV.M			
51) Sample	90	M2015-3237-2-BNBLK	Lab No.: M2015-3237-2
52) Sample	11	M2015-3237-2-BNr	Lab No.: M2015-3237-2
53) Sample	89	M2015-3267-1-BNBLK	Lab No.: M2015-3267-1
54) Sample	12	M2015-3267-1-BNr	Lab No.: M2015-3267-1
55) Sample	88	M2015-3274-1-BNBLK	Lab No.: M2015-3274-1
56) Sample	13	M2015-3274-1-BNr	Lab No.: M2015-3274-1
57) Sample	87	M2015-3276-1-BNBLK	Lab No.: M2015-3276-1
58) Sample	14	M2015-3276-1-BNr	Lab No.: M2015-3276-1
59) Sample	86	M2015-3289-1-BNBLK	Lab No.: M2015-3289-1
60) Sample	15	M2015-3289-1-BNr	Lab No.: M2015-3289-1
Acquisition Method: BNSB120510.M			
61) Sample	85	M2015-3336-2-BNBLK	Lab No.: M2015-3336-2
62) Sample	16	M2015-3336-2-BN	Lab No.: M2015-3336-2
63) Sample	84	M2015-3360-1-BNBLK	Lab No.: M2015-3360-1
64) Sample	17	M2015-3360-1-BN	Lab No.: M2015-3360-1
65) Sample	83	M2015-3361-1-BNBLK	Lab No.: M2015-3361-1
66) Sample	18	M2015-3361-1-BN	Lab No.: M2015-3361-1
67) Sample	82	M2015-3377-1-BNBLK	Lab No.: M2015-3377-1
68) Sample	19	M2015-3377-1-BN	Lab No.: M2015-3377-1
69) Sample	81	M2015-3402-2-BNBLK	Lab No.: M2015-3402-2
70) Sample	20	M2015-3402-2-BN	Lab No.: M2015-3402-2
Acquisition Method: GBT092509-Delta EMV.M			
71) Sample	85	M2015-3336-2-BNBLK	Lab No.: M2015-3336-2
72) Sample	16	M2015-3336-2-BNr	Lab No.: M2015-3336-2
73) Sample	84	M2015-3360-1-BNBLK	Lab No.: M2015-3360-1
74) Sample	17	M2015-3360-1-BNr	Lab No.: M2015-3360-1
75) Sample	83	M2015-3361-1-BNBLK	Lab No.: M2015-3361-1
76) Sample	18	M2015-3361-1-BN	Lab No.: M2015-3361-1
77) Sample	82	M2015-3377-1-BNBLK	Lab No.: M2015-3377-1
78) Sample	19	M2015-3377-1-BNr	Lab No.: M2015-3377-1
79) Sample	81	M2015-3402-2-BNBLK	Lab No.: M2015-3402-2
80) Sample	20	M2015-3402-2-BNr	Lab No.: M2015-3402-2
Acquisition Method: BNSB120510.M			
81) Sample	80	M2015-3424-3-BNBLK	Lab No.: M2015-3424-3
82) Sample	21	M2015-3424-3-BN	Lab No.: M2015-3424-3
83) Sample	79	P2015-2011-1-BNBLK	Lab No.: P2015-2011-1
84) Sample	22	P2015-2011-1-BN	Lab No.: P2015-2011-1
85) Sample	78	P2015-2017-1-BNBLK	Lab No.: P2015-2017-1
86) Sample	23	P2015-2017-1-BN	Lab No.: P2015-2017-1
87) Sample	77	P2015-2018-1-BNBLK	Lab No.: P2015-2018-1
88) Sample	24	P2015-2018-1-BN	Lab No.: P2015-2018-1
89) Sample	76	P2015-2025-1-BNBLK	Lab No.: P2015-2025-1
90) Sample	25	P2015-2025-1-BN	Lab No.: P2015-2025-1
Acquisition Method: GBT092509-Delta EMV.M			
91) Sample	80	M2015-3424-3-BNBLK	Lab No.: M2015-3424-3
92) Sample	21	M2015-3424-3-BNr	Lab No.: M2015-3424-3
93) Sample	79	P2015-2011-1-BNBLK	Lab No.: P2015-2011-1
94) Sample	22	P2015-2011-1-BNr	Lab No.: P2015-2011-1
95) Sample	78	P2015-2017-1-BNBLK	Lab No.: P2015-2017-1
96) Sample	23	P2015-2017-1-BNr	Lab No.: P2015-2017-1
97) Sample	77	P2015-2018-1-BNBLK	Lab No.: P2015-2018-1
98) Sample	24	P2015-2018-1-BNr	Lab No.: P2015-2018-1
99) Sample	76	P2015-2025-1-BNBLK	Lab No.: P2015-2025-1
100) Sample	25	P2015-2025-1-BNr	Lab No.: P2015-2025-1
Acquisition Method: BNSB120510.M			



simulate_sequence.log

101) Sample	75	P2015-2033-1-BNBLK	Lab No.:	P2015-2033-1
102) Sample	26	P2015-2033-1-BN	Lab No.:	P2015-2033-1
103) Sample	74	P2015-2034-1-BNBLK	Lab No.:	P2015-2034-1
104) Sample	27	P2015-2034-1-BN	Lab No.:	P2015-2034-1
105) Sample	73	P2015-2068-1-BNBLK	Lab No.:	P2015-2068-1
106) Sample	28	P2015-2068-1-BN	Lab No.:	P2015-2068-1
107) Sample	72	P2015-2083-1-BNBLK	Lab No.:	P2015-2083-1
108) Sample	29	P2015-2083-1-BN	Lab No.:	P2015-2083-1
109) Sample	71	P2015-2084-1-BNBLK	Lab No.:	P2015-2084-1
110) Sample	30	P2015-2084-1-BN	Lab No.:	P2015-2084-1

Acquisition Method: GBT092509-Delta EMV.M

111) Sample	75	P2015-2033-1-BNBLKr	Lab No.:	P2015-2033-1
112) Sample	26	P2015-2033-1-BNr	Lab No.:	P2015-2033-1
113) Sample	74	P2015-2034-1-BNBLKr	Lab No.:	P2015-2034-1
114) Sample	27	P2015-2034-1-BNr	Lab No.:	P2015-2034-1
115) Sample	73	P2015-2068-1-BNBLKr	Lab No.:	P2015-2068-1
116) Sample	28	P2015-2068-1-BNr	Lab No.:	P2015-2068-1
117) Sample	72	P2015-2083-1-BNBLKr	Lab No.:	P2015-2083-1
118) Sample	29	P2015-2083-1-BNr	Lab No.:	P2015-2083-1
119) Sample	71	P2015-2084-1-BNBLKr	Lab No.:	P2015-2084-1
120) Sample	30	P2015-2084-1-BNr	Lab No.:	P2015-2084-1

Acquisition Method: BNSB120510.M

121) Sample	70	P2015-2089-1-BNBLK	Lab No.:	P2015-2089-1
122) Sample	31	P2015-2089-1-BN	Lab No.:	P2015-2089-1
123) Sample	69	P2015-2092-1-BNBLK	Lab No.:	P2015-2092-1
124) Sample	32	P2015-2092-1-BN	Lab No.:	P2015-2092-1
125) Sample	68	P2015-2093-1-BNBLK	Lab No.:	P2015-2093-1
126) Sample	33	P2015-2093-1-BN	Lab No.:	P2015-2093-1
127) Sample	67	P2015-2096-1-BNBLK	Lab No.:	P2015-2096-1
128) Sample	34	P2015-2096-1-BN	Lab No.:	P2015-2096-1
129) Sample	66	P2015-2097-1-BNBLK	Lab No.:	P2015-2097-1
130) Sample	35	P2015-2097-1-BN	Lab No.:	P2015-2097-1

Acquisition Method: GBT092509-Delta EMV.M

131) Sample	70	P2015-2089-1-BNBLKr	Lab No.:	P2015-2089-1
132) Sample	31	P2015-2089-1-BNr	Lab No.:	P2015-2089-1
133) Sample	69	P2015-2092-1-BNBLKr	Lab No.:	P2015-2092-1
134) Sample	32	P2015-2092-1-BNr	Lab No.:	P2015-2092-1
135) Sample	68	P2015-2093-1-BNBLKr	Lab No.:	P2015-2093-1
136) Sample	33	P2015-2093-1-BNr	Lab No.:	P2015-2093-1
137) Sample	67	P2015-2096-1-BNBLKr	Lab No.:	P2015-2096-1
138) Sample	34	P2015-2096-1-BNr	Lab No.:	P2015-2096-1
139) Sample	66	P2015-2097-1-BNBLKr	Lab No.:	P2015-2097-1
140) Sample	35	P2015-2097-1-BNr	Lab No.:	P2015-2097-1

Acquisition Method: BNSB120510.M

141) Sample	65	P2015-2113-1-BNBLK	Lab No.:	P2015-2113-1
142) Sample	36	P2015-2113-1-BN	Lab No.:	P2015-2113-1
143) Sample	64	P2015-2123-1-BNBLK	Lab No.:	P2015-2123-1
144) Sample	37	P2015-2123-1-BN	Lab No.:	P2015-2123-1
145) Sample	63	P2015-2129-1-BNBLK	Lab No.:	P2015-2129-1
146) Sample	38	P2015-2129-1-BN	Lab No.:	P2015-2129-1
147) Sample	62	P2015-2161-1-BNBLK	Lab No.:	P2015-2161-1
148) Sample	39	P2015-2161-1-BN	Lab No.:	P2015-2161-1
149) Sample	61	P2015-2162-1-BNBLK	Lab No.:	P2015-2162-1
150) Sample	40	P2015-2162-1-BN	Lab No.:	P2015-2162-1

Acquisition Method: GBT092509-Delta EMV.M

151) Sample	65	P2015-2113-1-BNBLKr	Lab No.:	P2015-2113-1
152) Sample	36	P2015-2113-1-BNr	Lab No.:	P2015-2113-1
153) Sample	64	P2015-2123-1-BNBLKr	Lab No.:	P2015-2123-1
154) Sample	37	P2015-2123-1-BNr	Lab No.:	P2015-2123-1
155) Sample	63	P2015-2129-1-BNBLKr	Lab No.:	P2015-2129-1
156) Sample	38	P2015-2129-1-BNr	Lab No.:	P2015-2129-1
157) Sample	62	P2015-2161-1-BNBLKr	Lab No.:	P2015-2161-1
158) Sample	39	P2015-2161-1-BNr	Lab No.:	P2015-2161-1



```
simulate_sequence.log
159) Sample      61      P2015-2162-1-BNBLKr  Lab No.: P2015-2162-1
160) Sample      40      P2015-2162-1-BNr    Lab No.: P2015-2162-1

Acquisition Method: BNSB120510.M
161) Sample      60      P2015-2184-1-BNBLK  Lab No.: P2015-2184-1
162) Sample      41      P2015-2184-1-BN     Lab No.: P2015-2184-1
163) Sample      59      P2015-2186-1-BNBLK  Lab No.: P2015-2186-1
164) Sample      42      P2015-2186-1-BN     Lab No.: P2015-2186-1
165) Sample      58      P2015-2194-1-BNBLK  Lab No.: P2015-2194-1
166) Sample      43      P2015-2194-1-BN     Lab No.: P2015-2194-1

Acquisition Method: GBT092509-Delta EMV.M
167) Sample      60      P2015-2184-1-BNBLKr  Lab No.: P2015-2184-1
168) Sample      41      P2015-2184-1-BNr    Lab No.: P2015-2184-1
169) Sample      59      P2015-2186-1-BNBLKr  Lab No.: P2015-2186-1
170) Sample      42      P2015-2186-1-BNr    Lab No.: P2015-2186-1
171) Sample      58      P2015-2194-1-BNBLKr  Lab No.: P2015-2194-1
172) Sample      43      P2015-2194-1-BNr    Lab No.: P2015-2194-1

Acquisition Method: BNSB120510.M
173) Sample      57      POSTBLKr             BLK

Acquisition Method: GBT092509-Delta EMV.M
174) Sample      56      AFTER                BLK
megabytes Needed: 3298 Space on drive D: 272609
Sequence Verification Done!
```

Analytical Method 3.6.1 & 3.6.7 QA Check List

Run Start Date: 10/02/15

Analyst: DND

(Short GC/MS temperature program)



Positive Control Compound List

- Phentermine (Cerilliant 30714-57F)
- Methamphetamine
- Nicotine
- Meperidine
- Caffeine
- Diphenhydramine
- Lidocaine
- PCP
- Methadone
- Amitriptyline
- Codeine
- Trazodone


Internal Standards

- Benzphetamine
- Papaverine

Optional back extraction **not** performed.
Samples reconstituted in methanol.




File :C:\gcms\1\data\Blood\100215\Prerun Solvent Blank.D
Operator : ISP\datastor
Acquired : 02 Oct 2015 23:55 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Pre-run Solvent Blank
Misc Info : Chloroform
Vial Number: 100


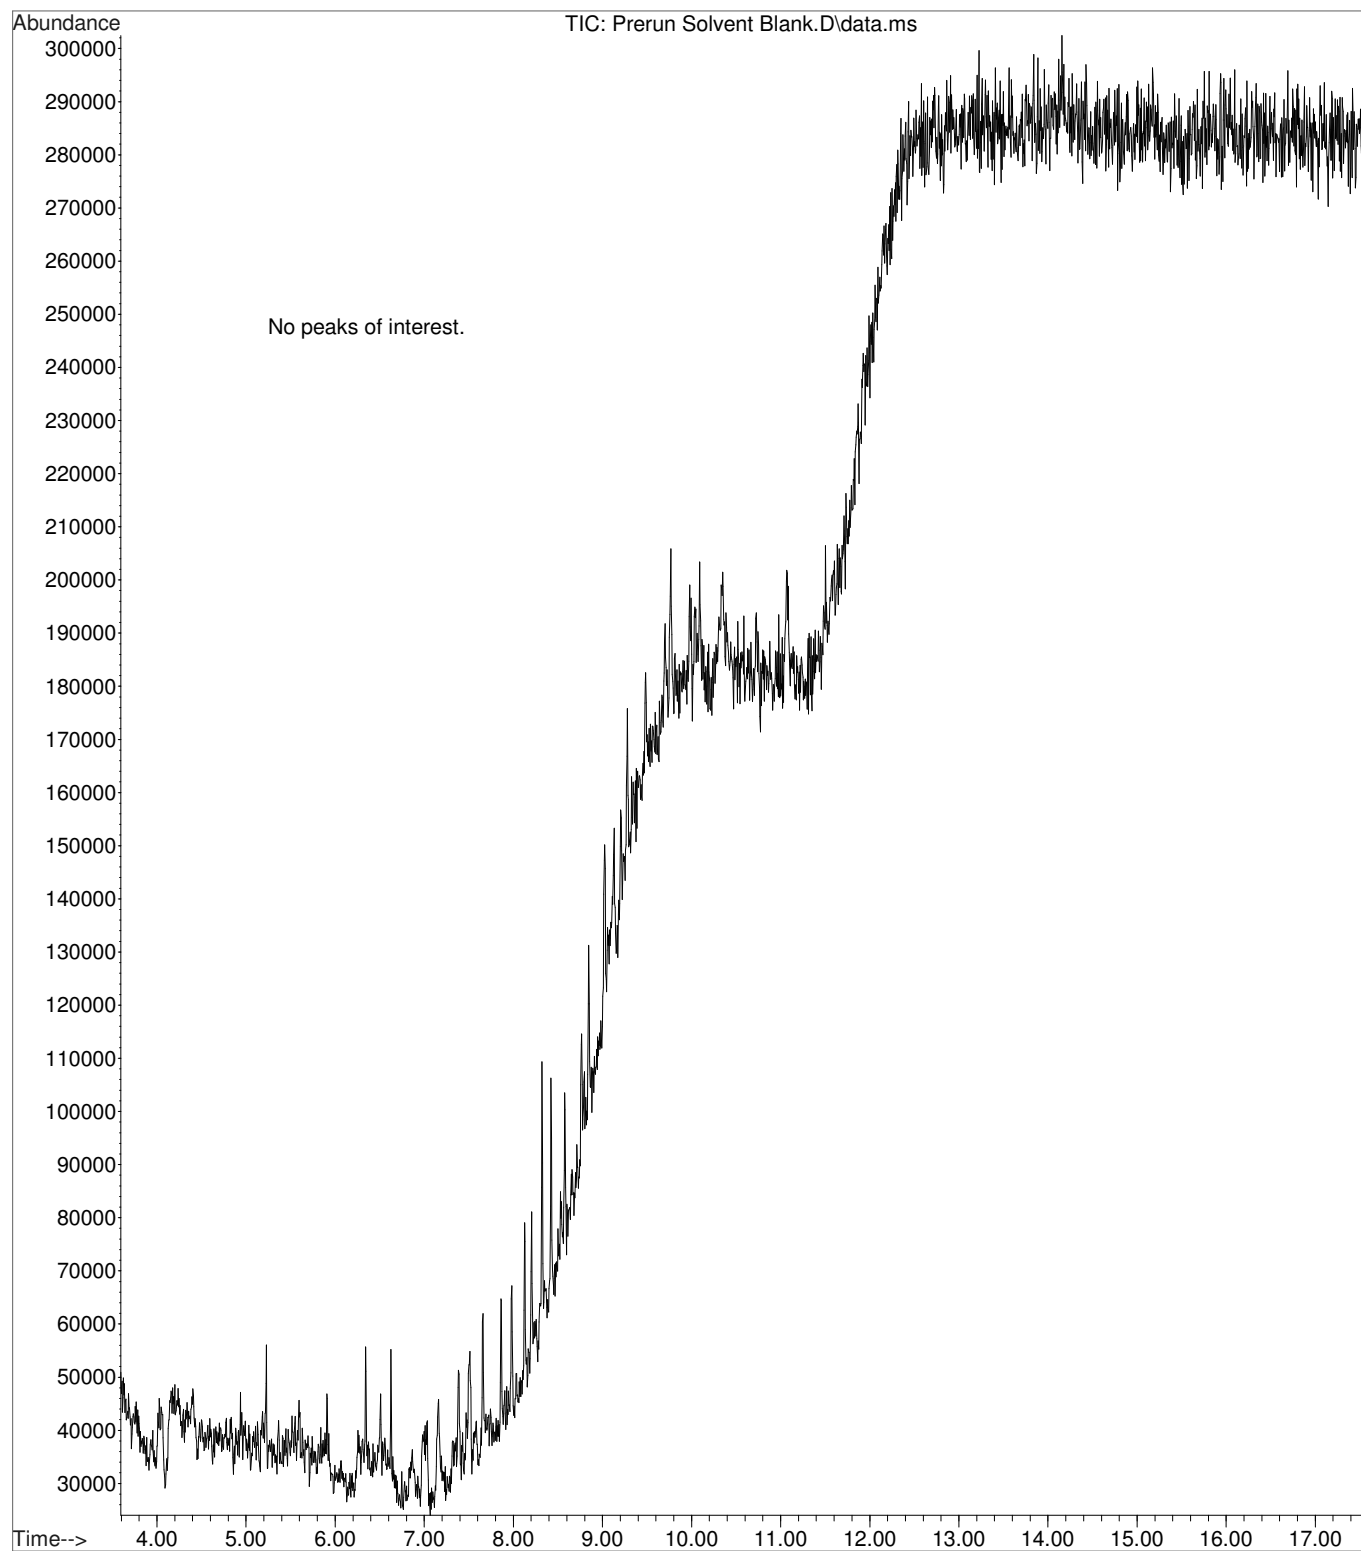







File :C:\gcms\1\data\Blood\100215\Negative Control-BN.D
Operator : ISP\datastor
Acquired : 03 Oct 2015 00:18 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1
Vial Number: 1

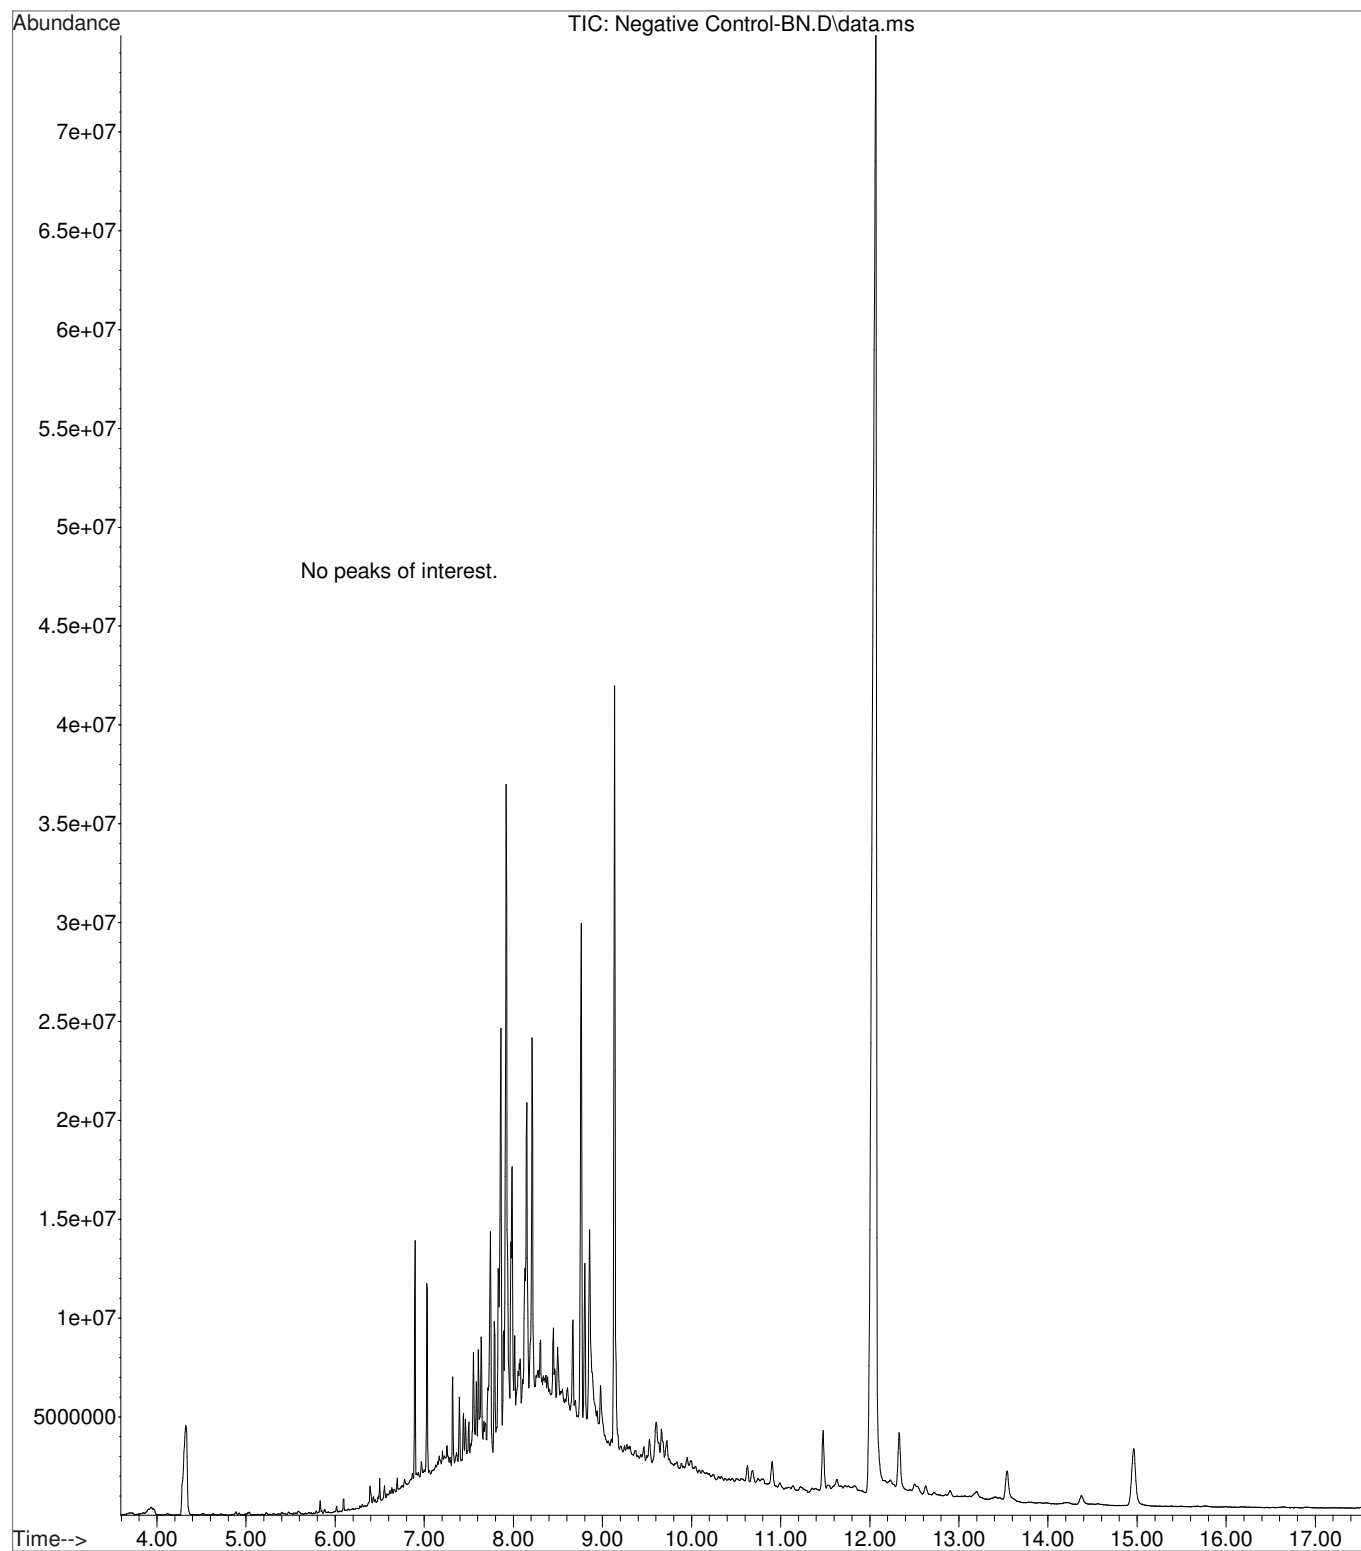


File :C:\gcms\1\data\Blood\100215\Negative Control-BN.D
Operator : ISP\datastor
Acquired : 03 Oct 2015 00:18 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1
Vial Number: 1

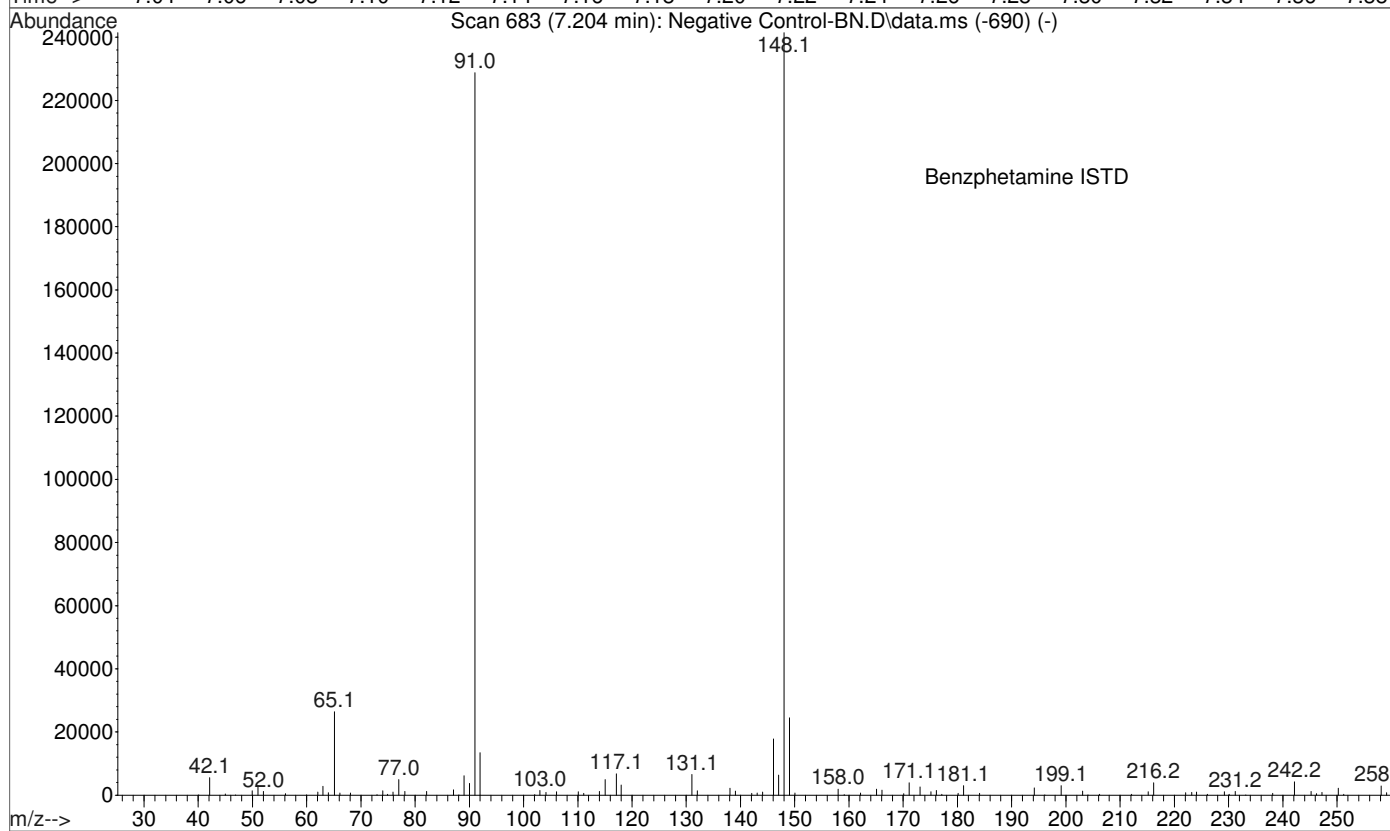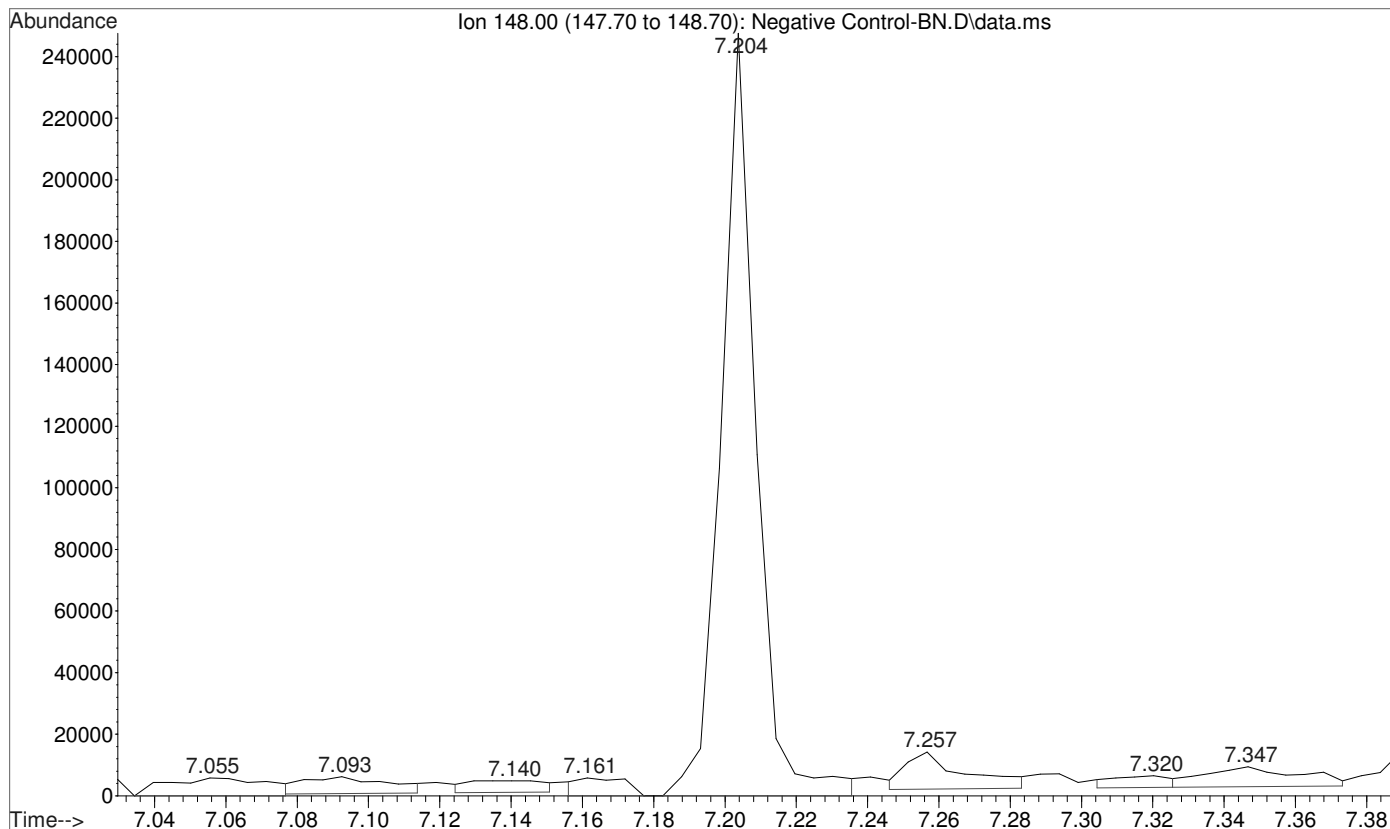


File :C:\gcms\1\data\Blood\100215\Negative Control-BN.D
Operator : ISP\datastor
Acquired : 03 Oct 2015 00:18 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1
Vial Number: 1

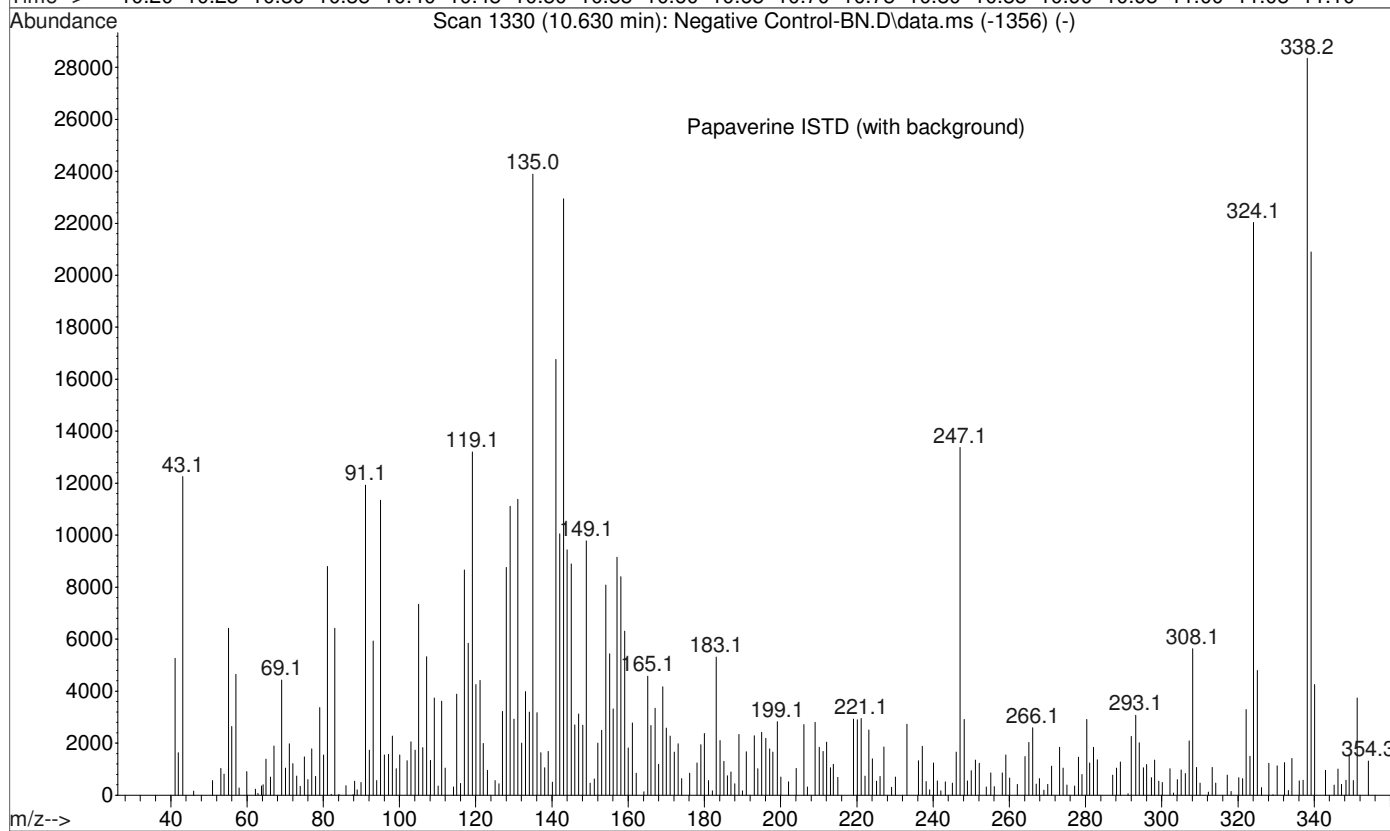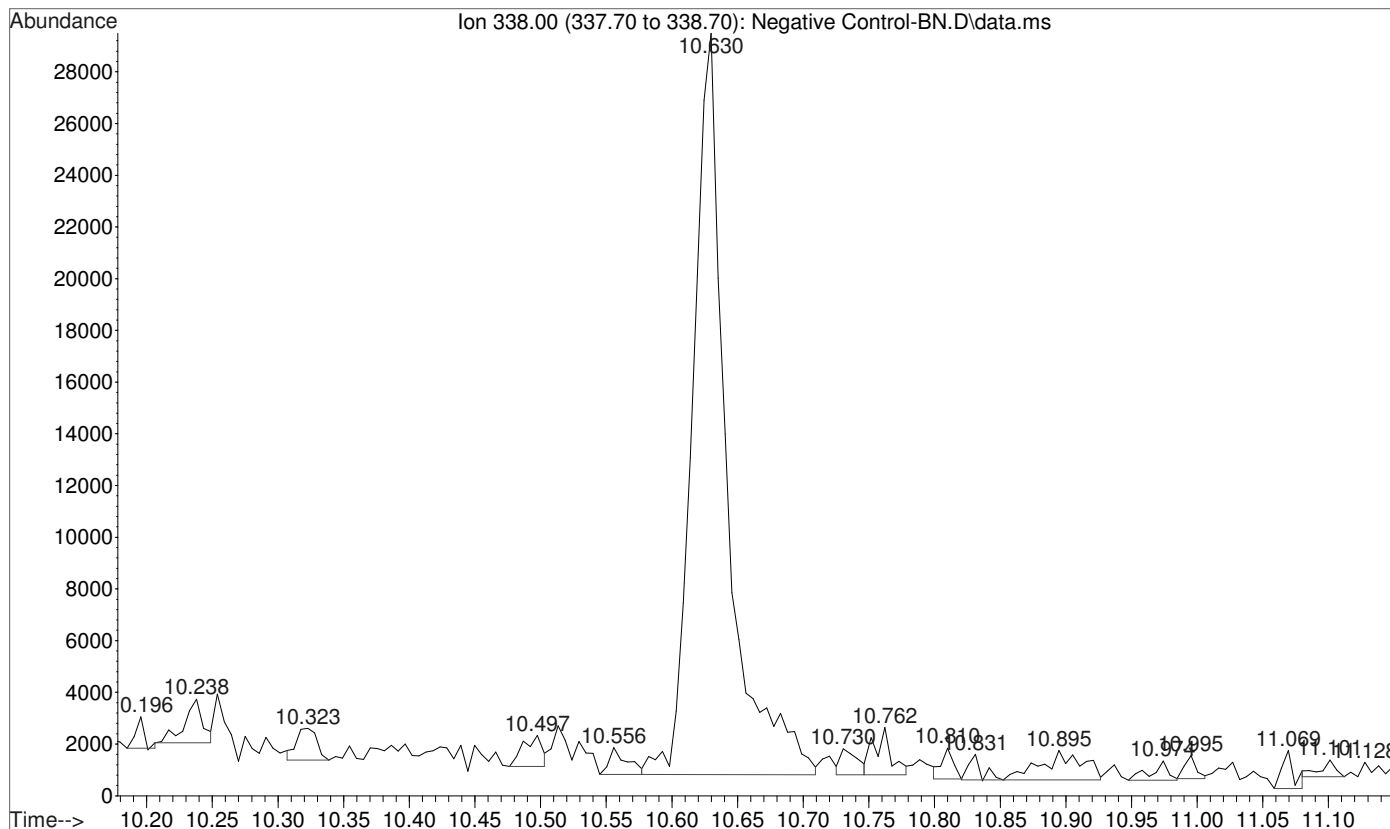







File :C:\gcms\1\data\Blood\100215\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 03 Oct 2015 00:41 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

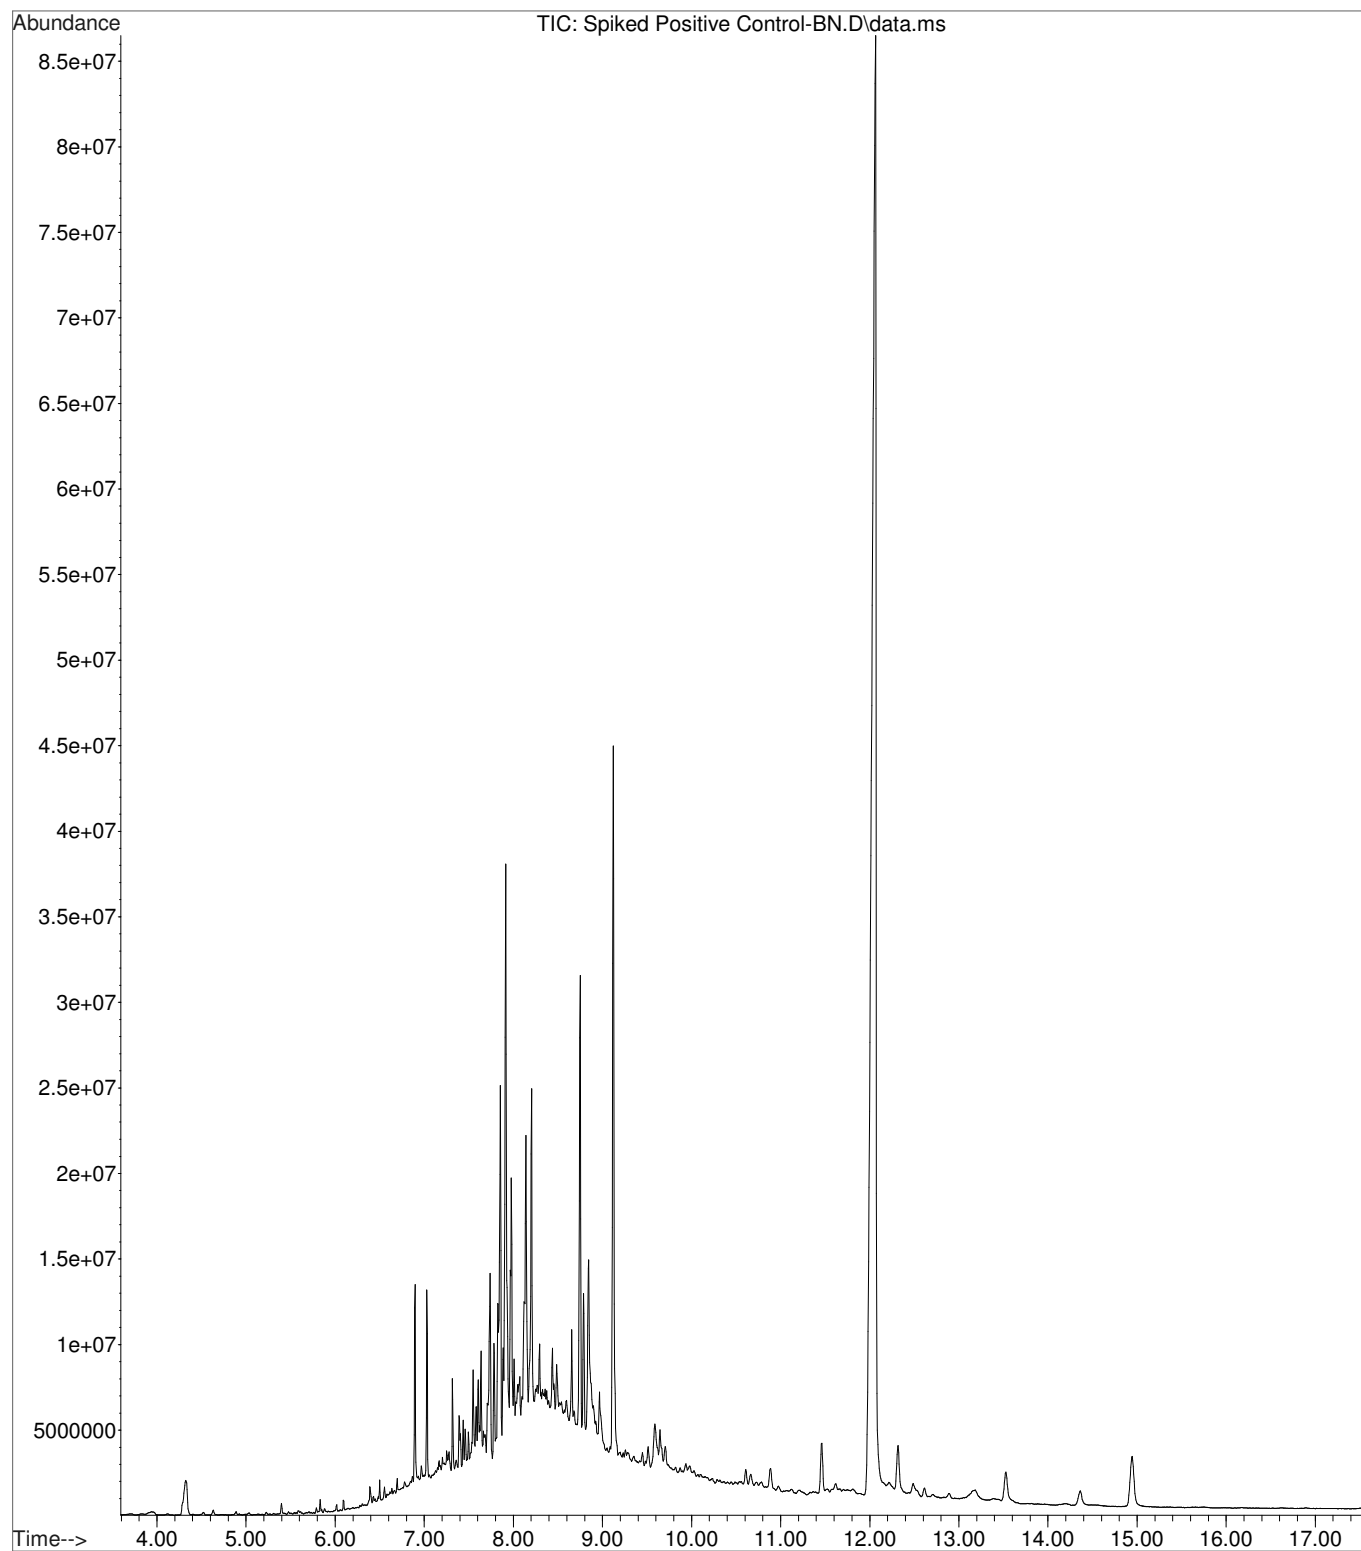



File :C:\gcms\1\data\Blood\100215\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 03 Oct 2015 00:41 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

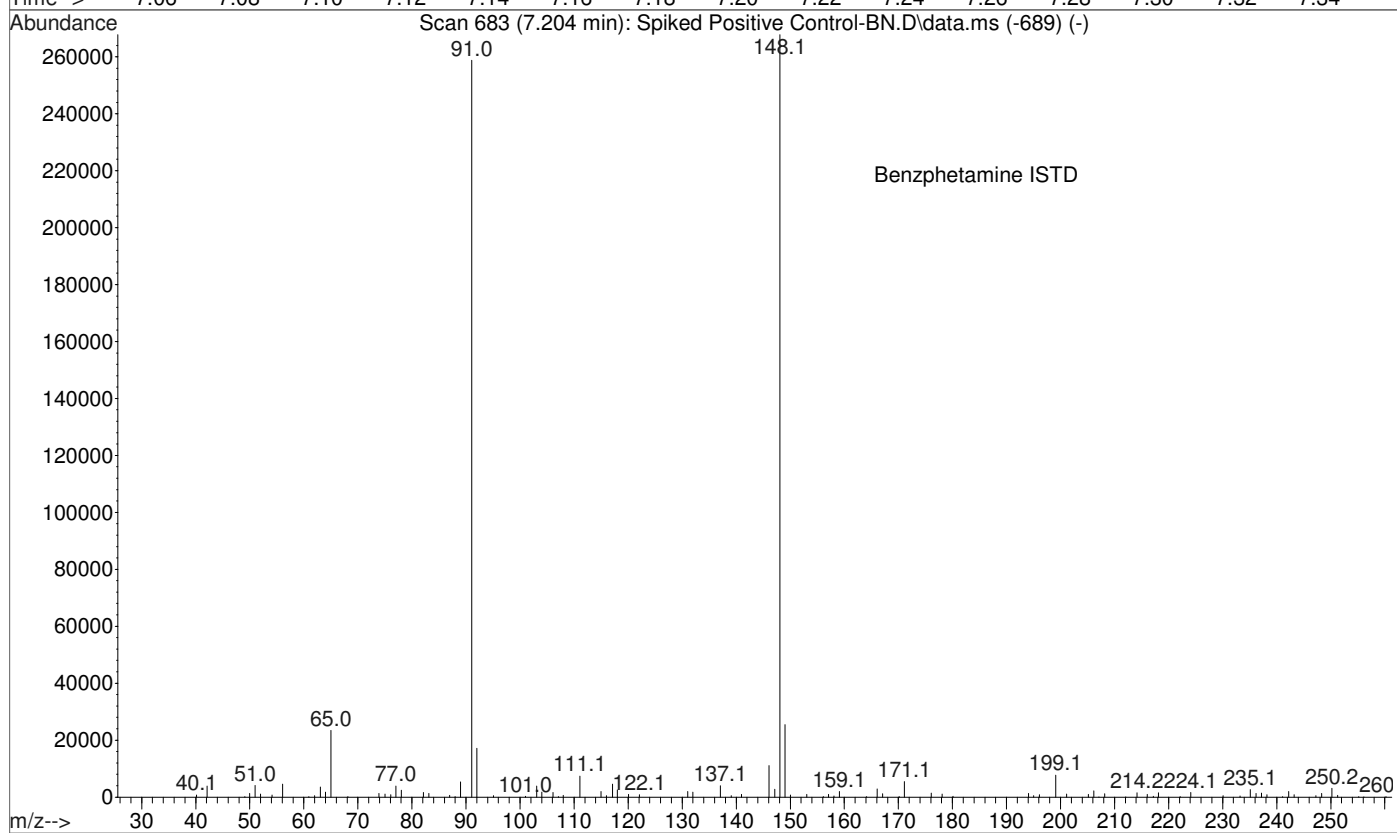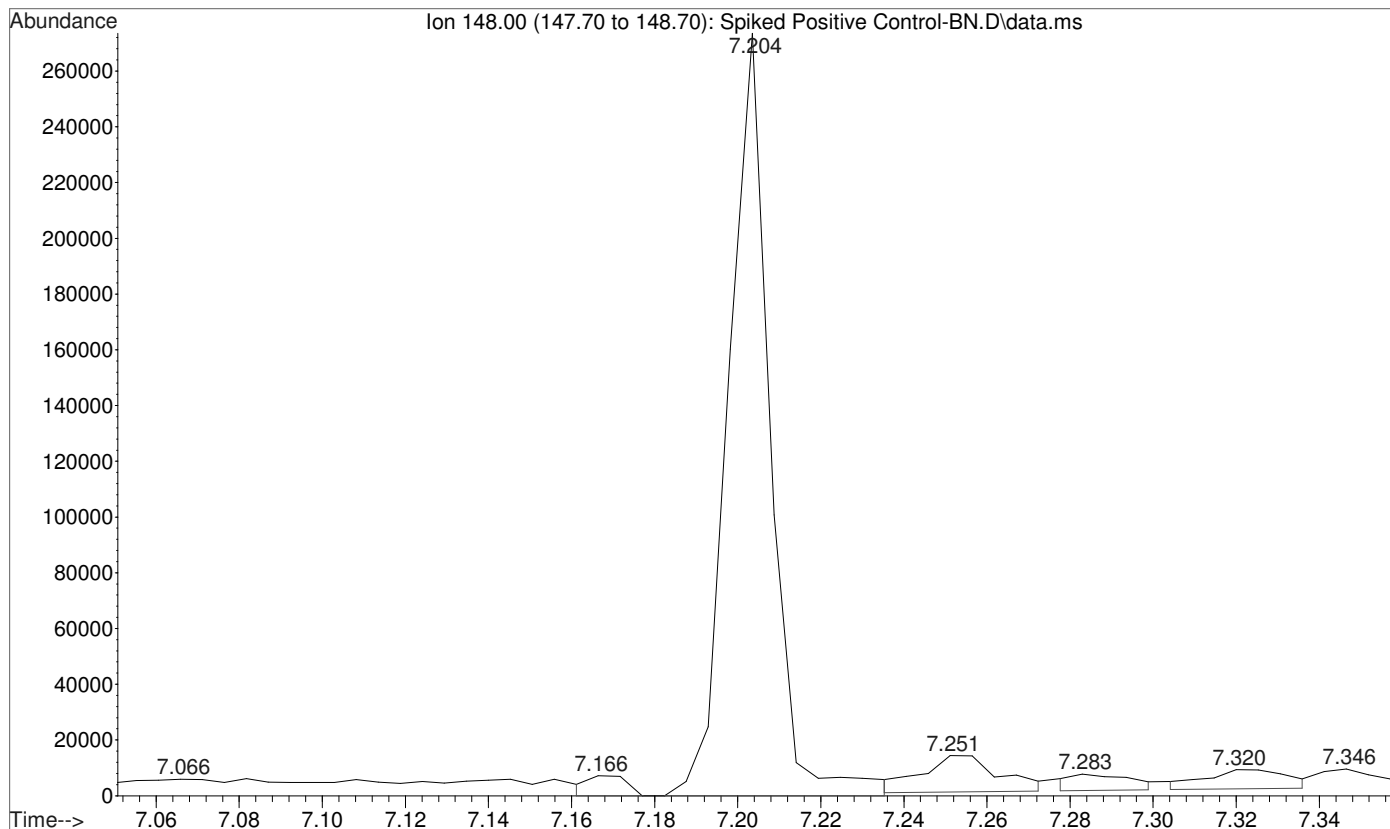



File :C:\gcms\1\data\Blood\100215\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 03 Oct 2015 00:41 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

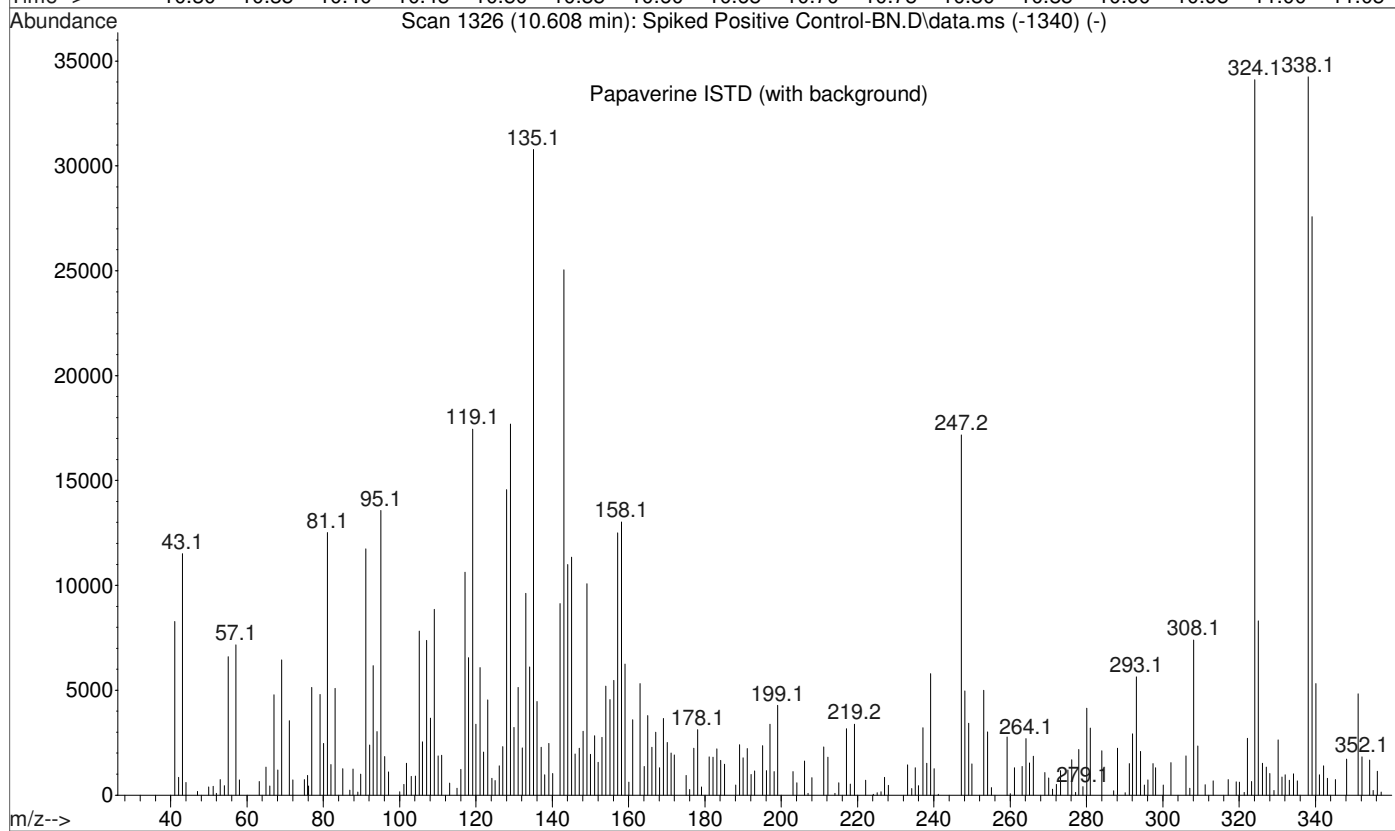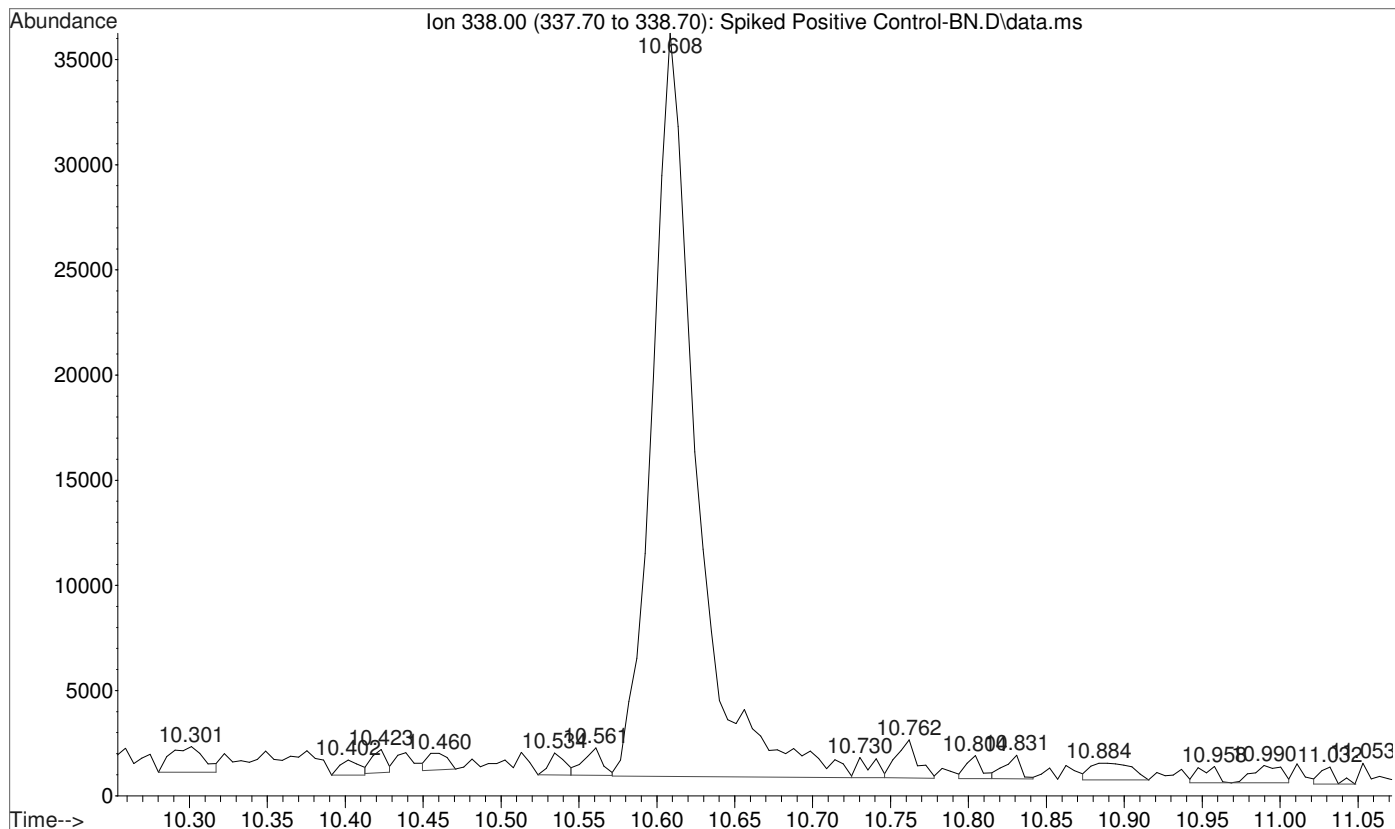



File :C:\gcms\1\data\Blood\100215\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 03 Oct 2015 00:41 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

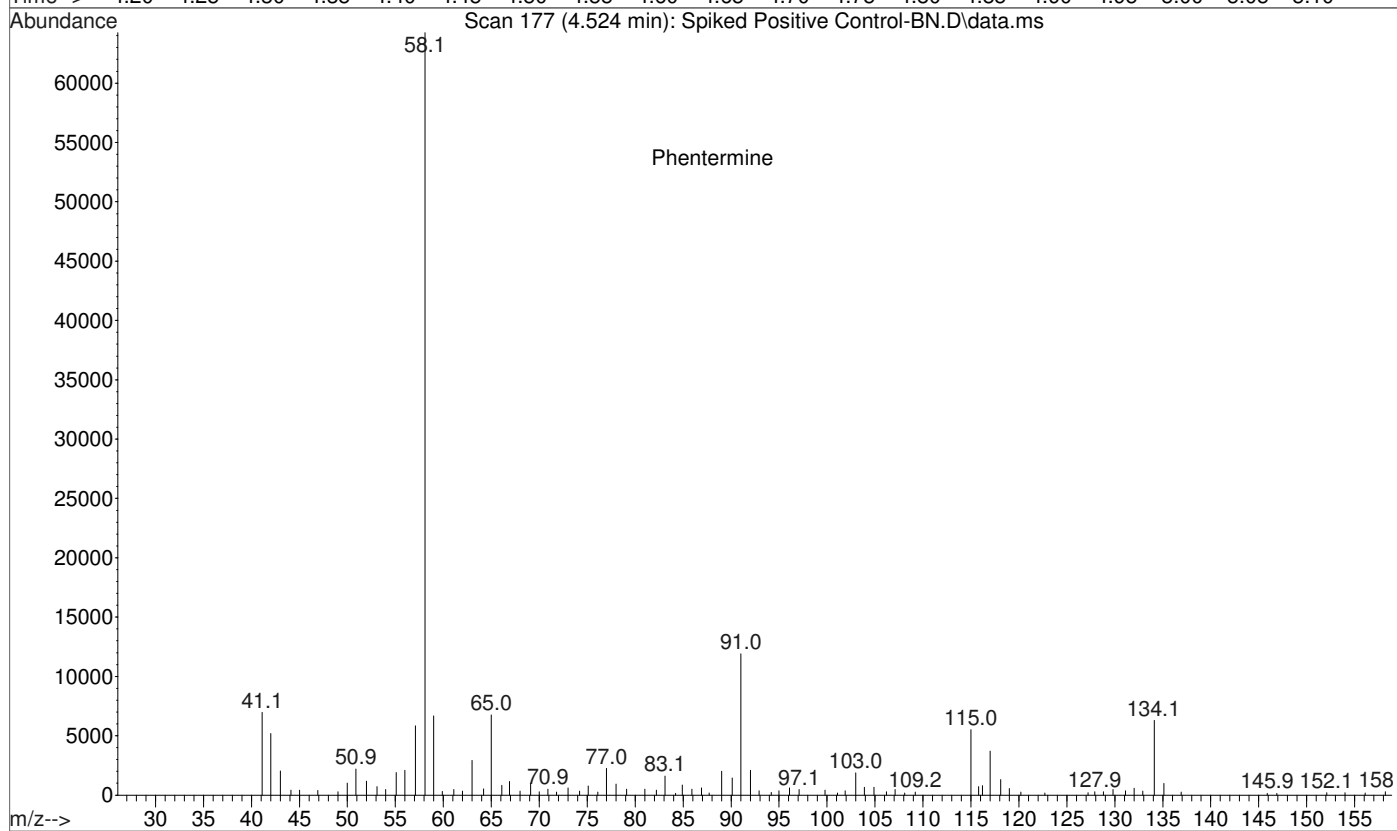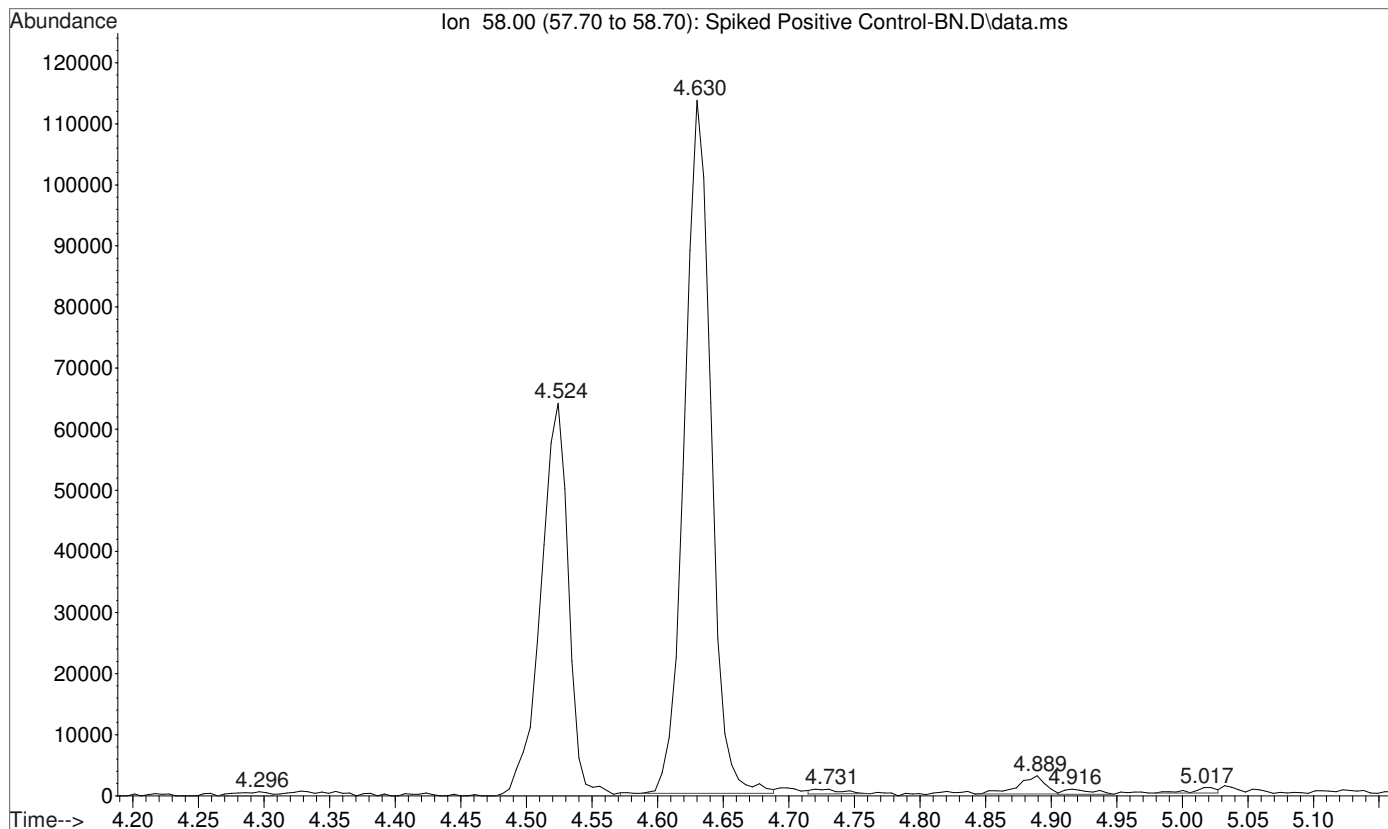



File :C:\gcms\1\data\Blood\100215\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 03 Oct 2015 00:41 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

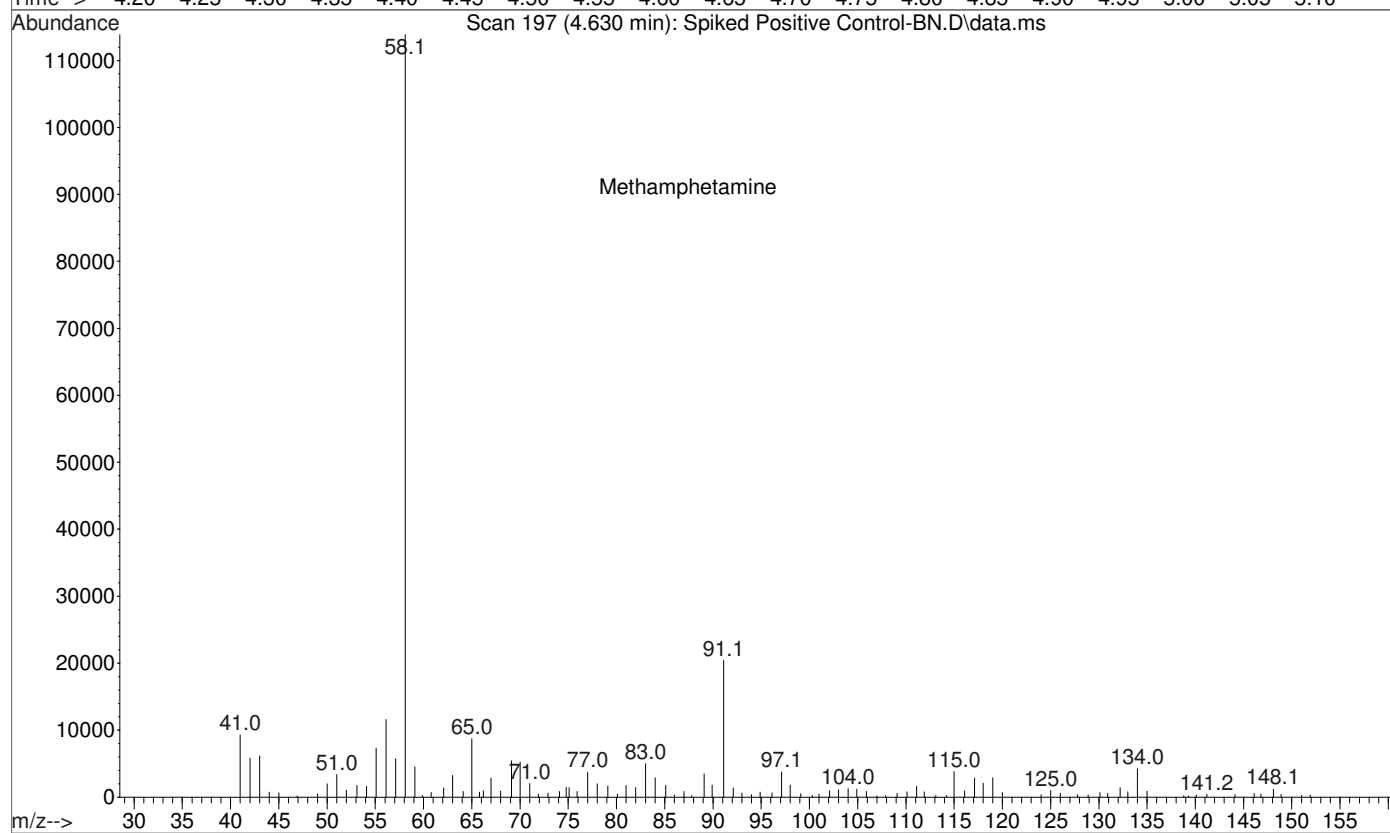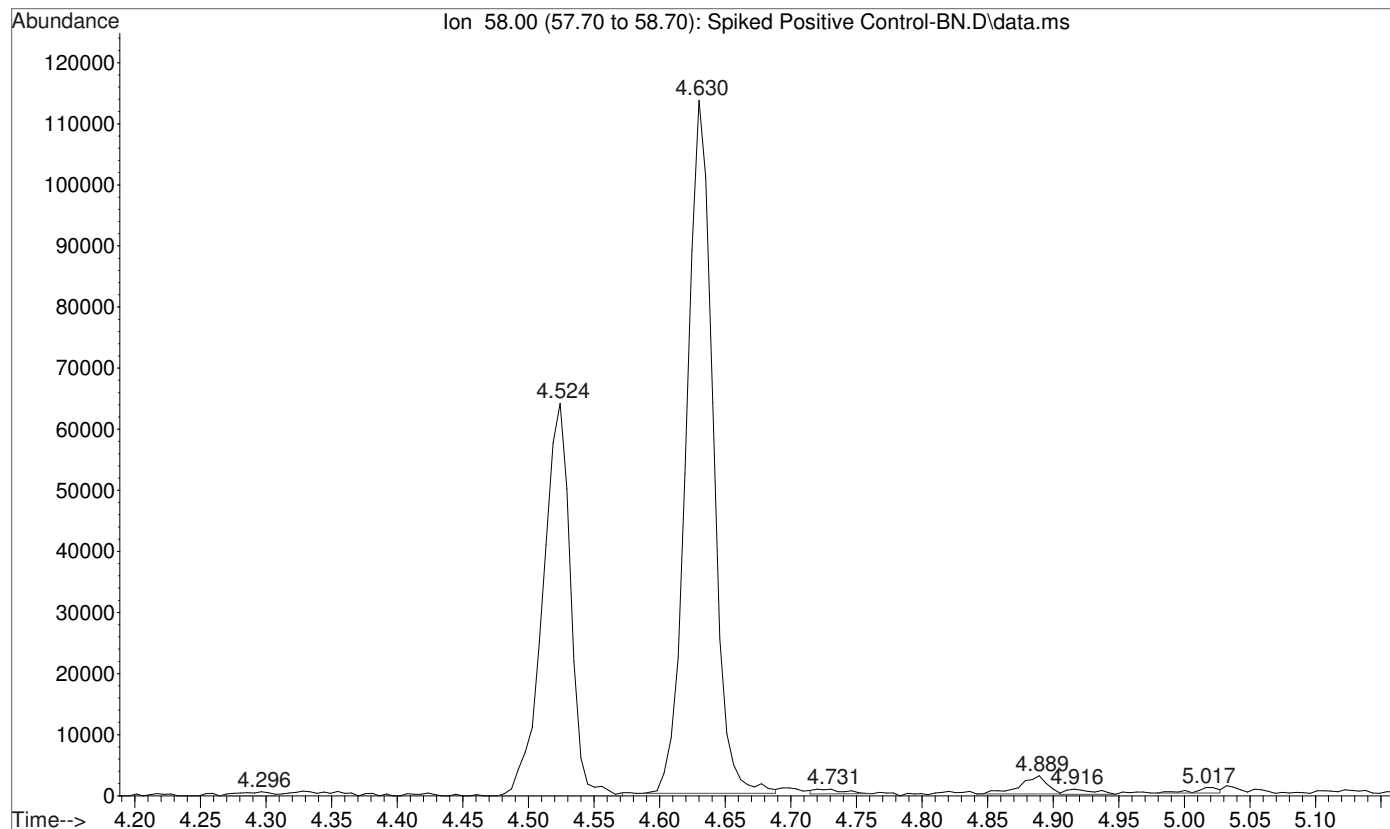



File :C:\gcms\1\data\Blood\100215\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 03 Oct 2015 00:41 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

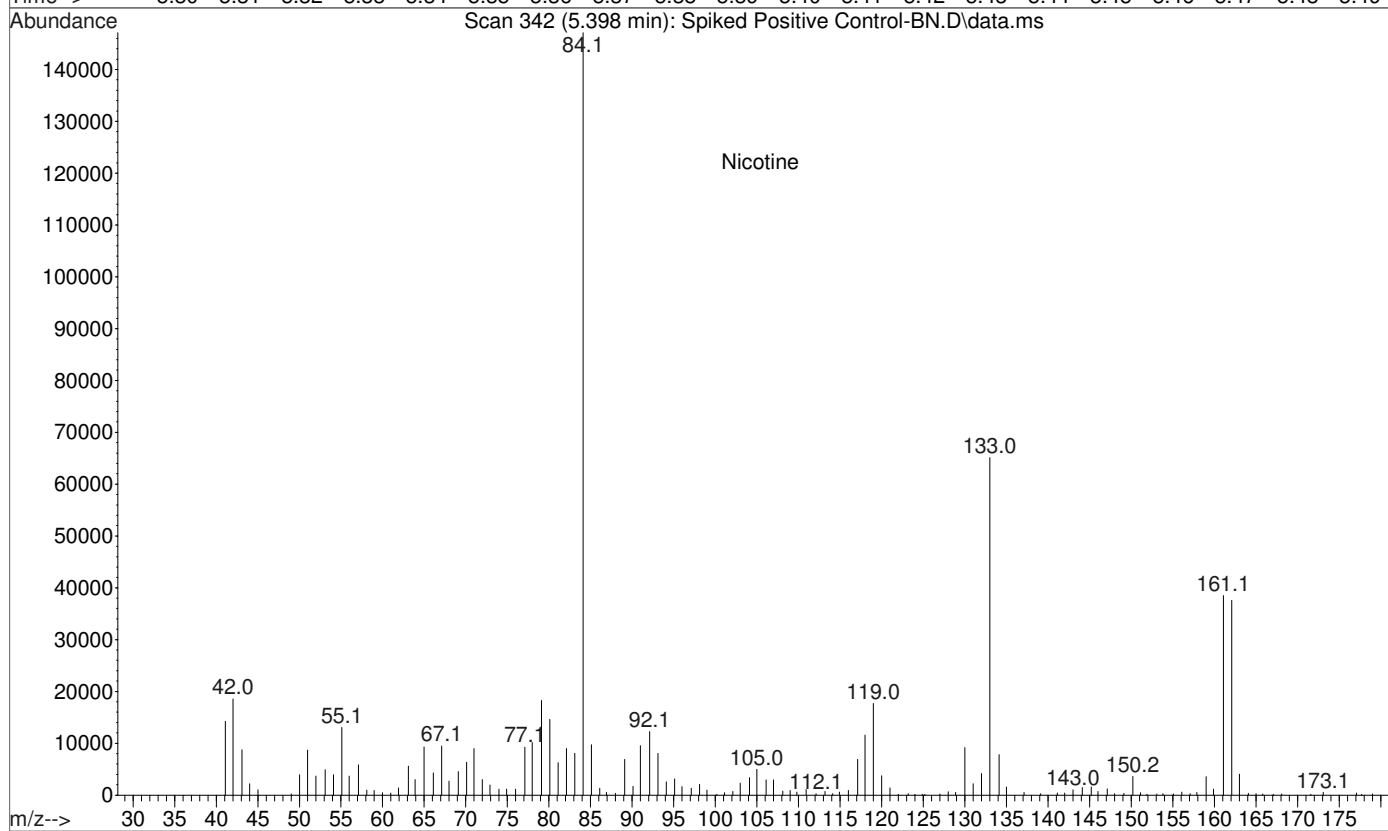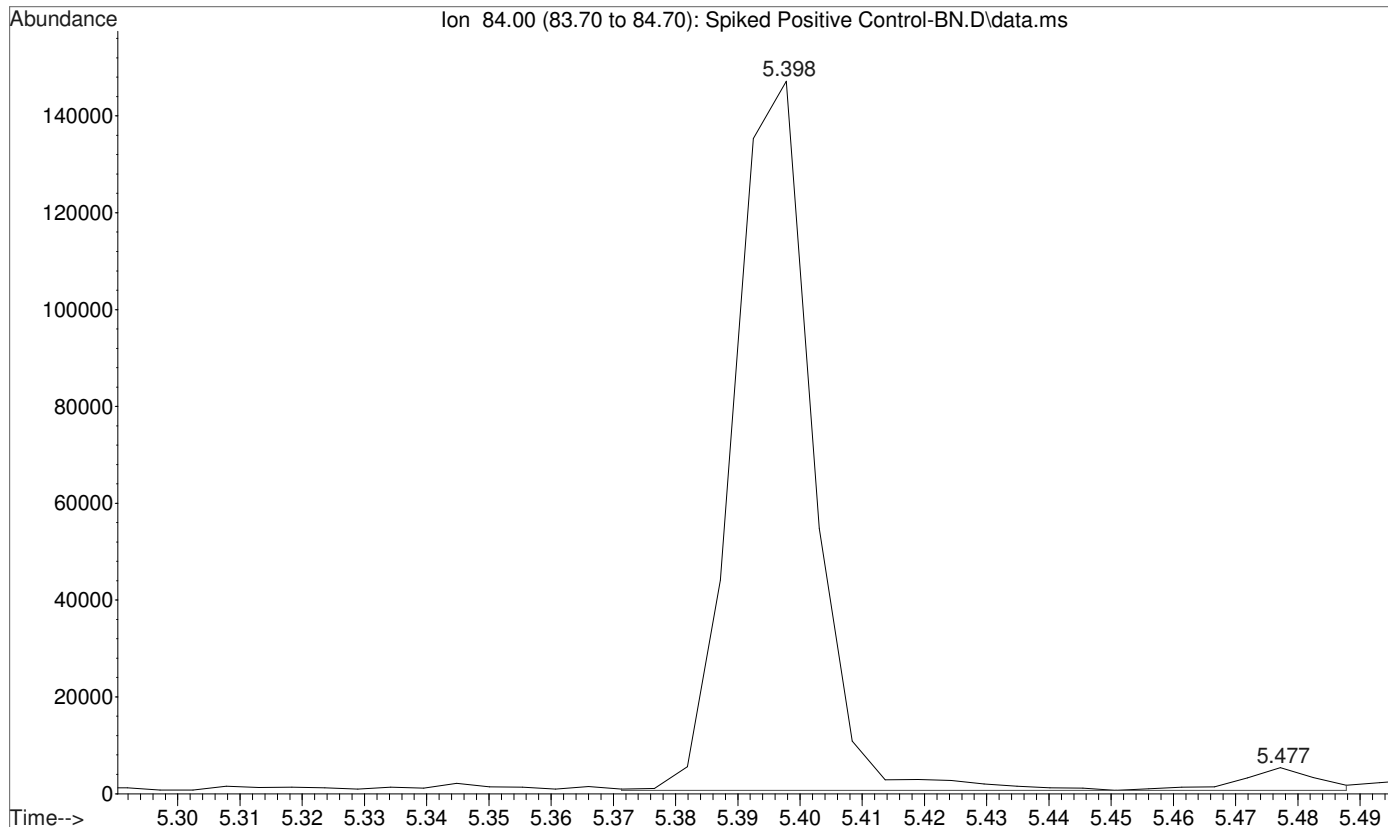



File :C:\gcms\1\data\Blood\100215\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 03 Oct 2015 00:41 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

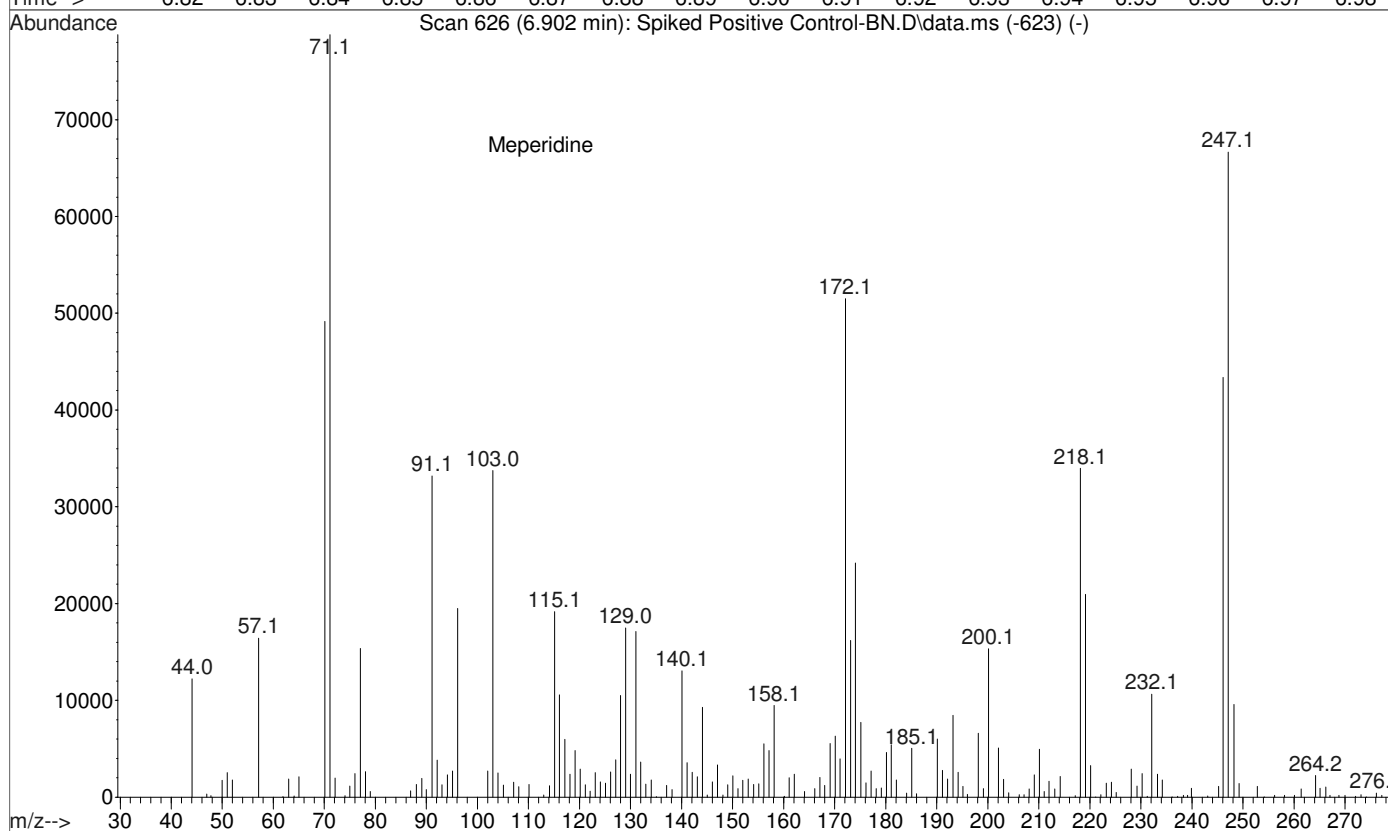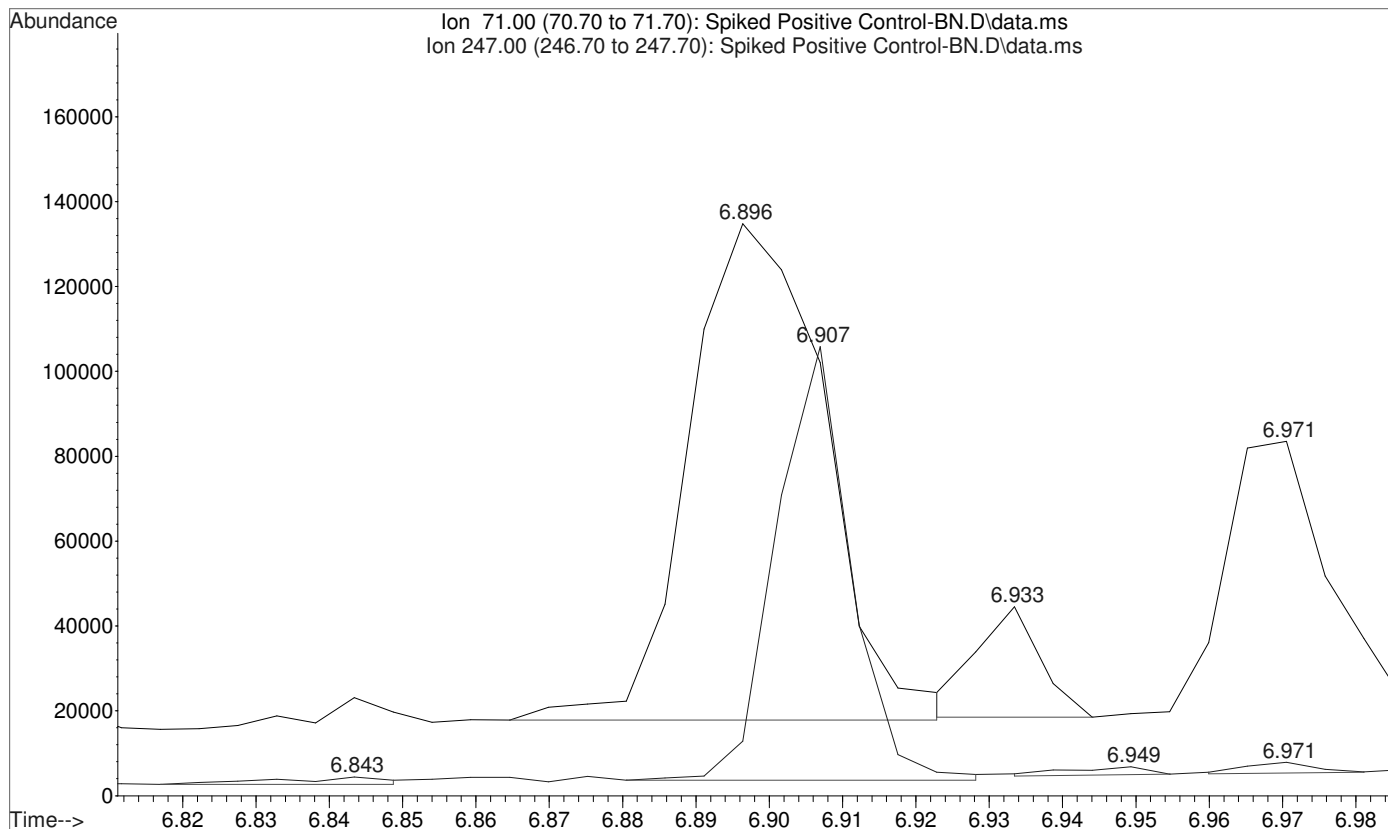



File :C:\gcms\1\data\Blood\100215\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 03 Oct 2015 00:41 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

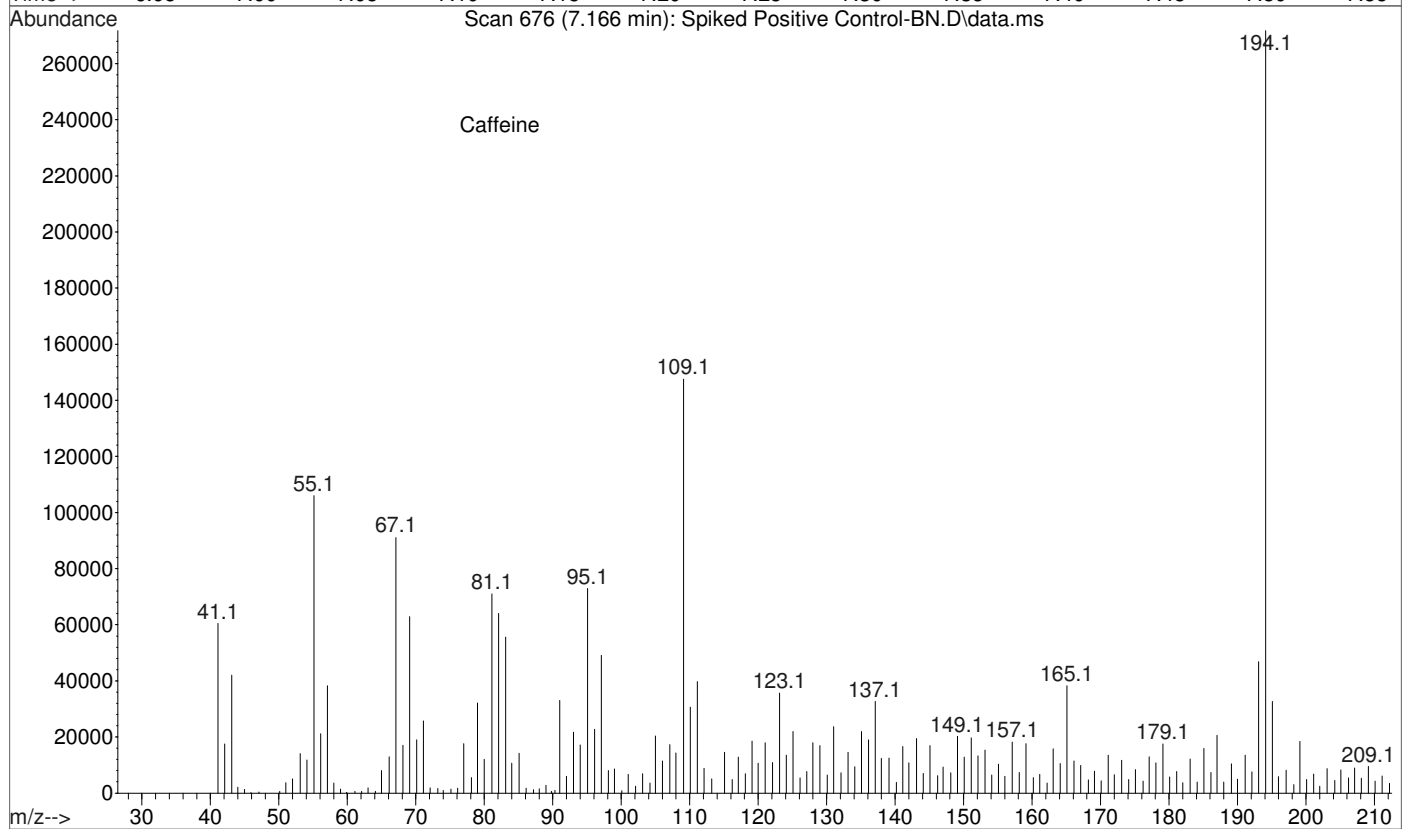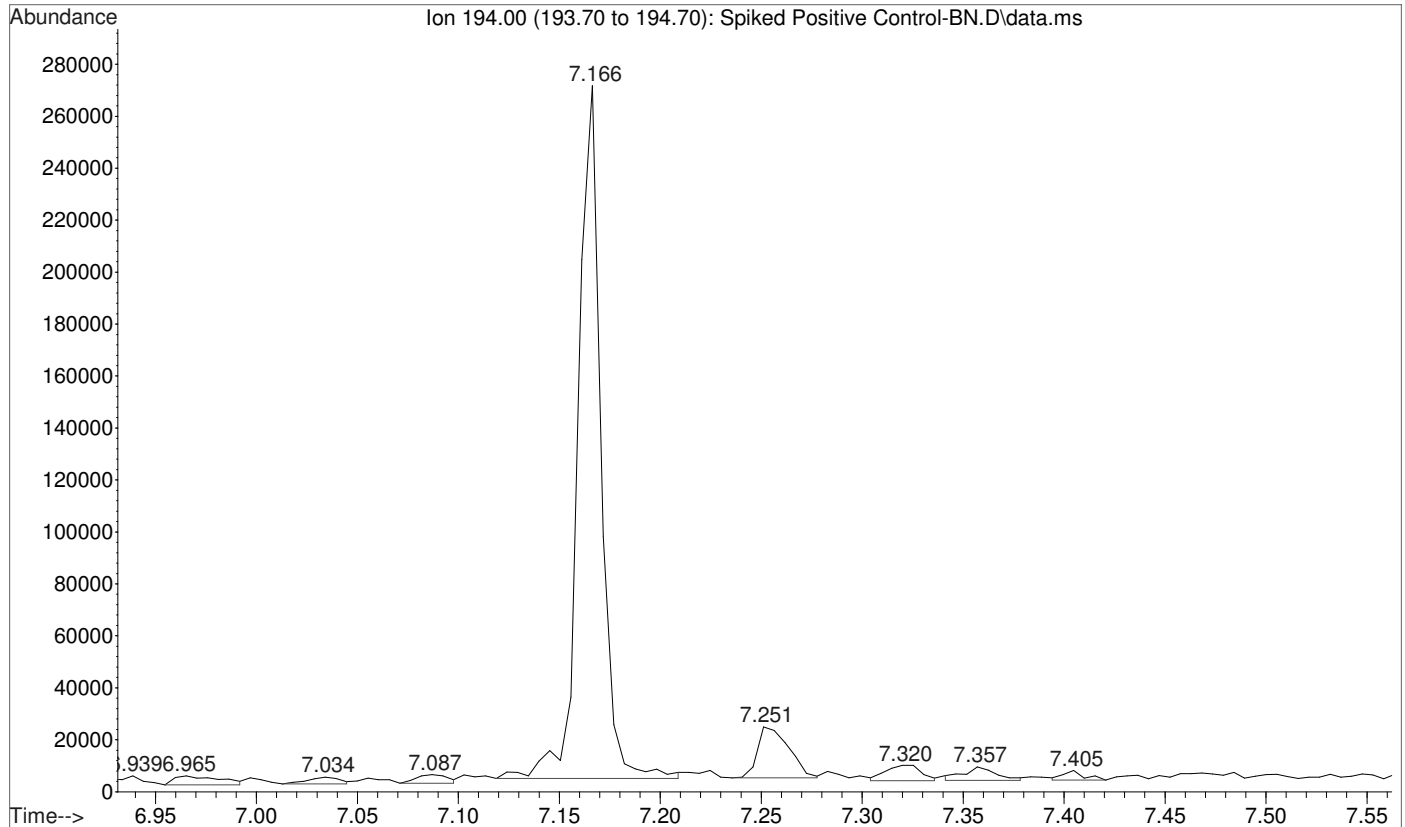



File :C:\gcms\1\data\Blood\100215\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 03 Oct 2015 00:41 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

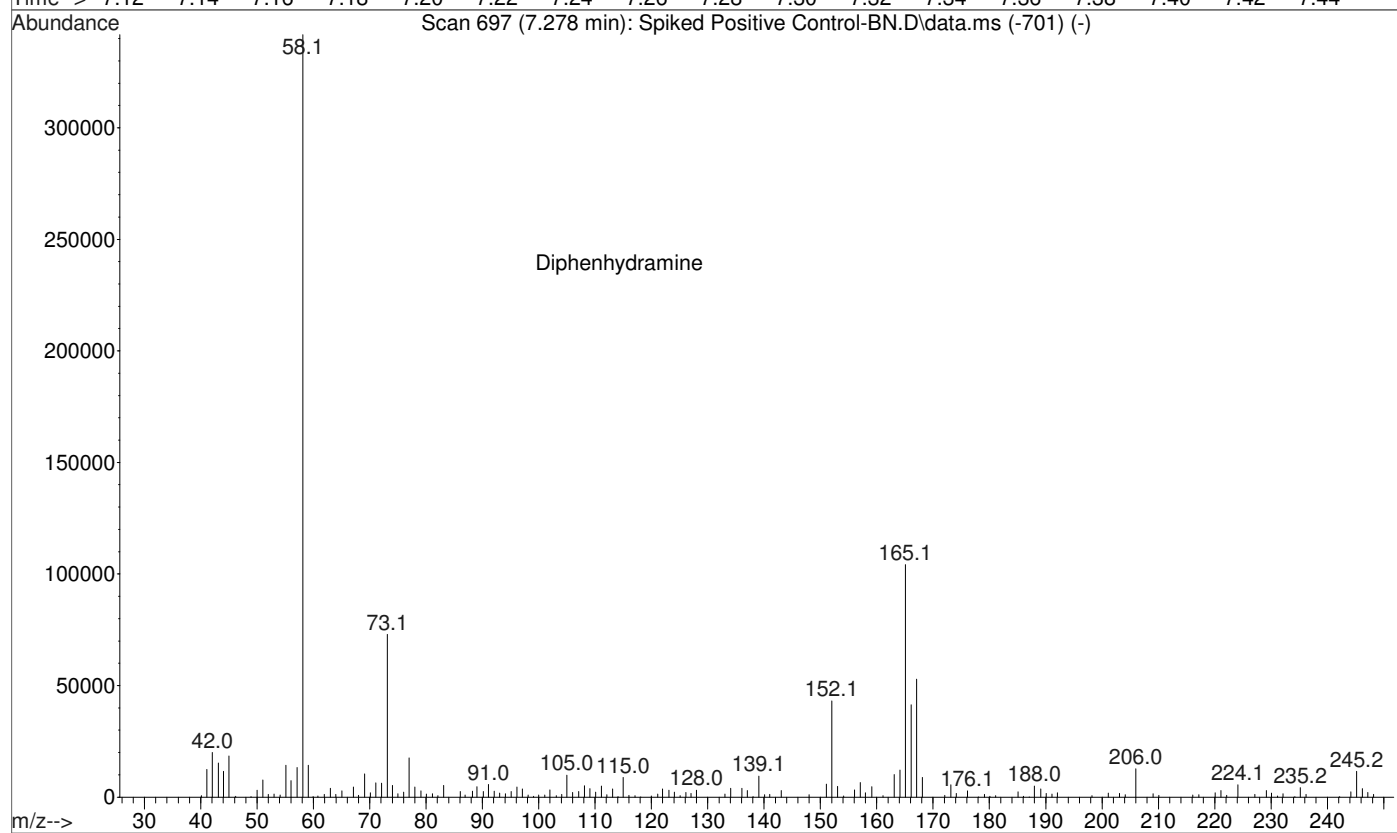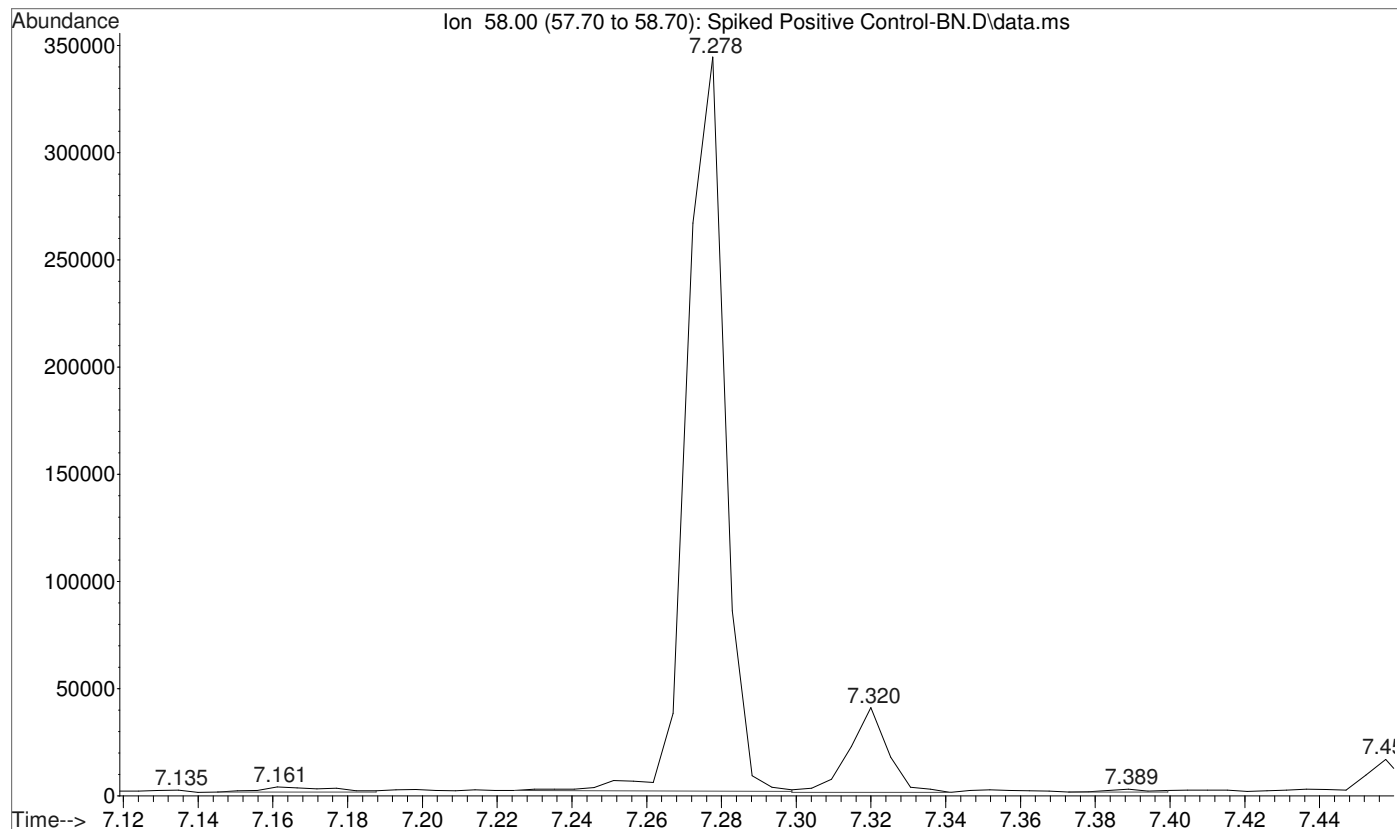




File :C:\gcms\1\data\Blood\100215\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 03 Oct 2015 00:41 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

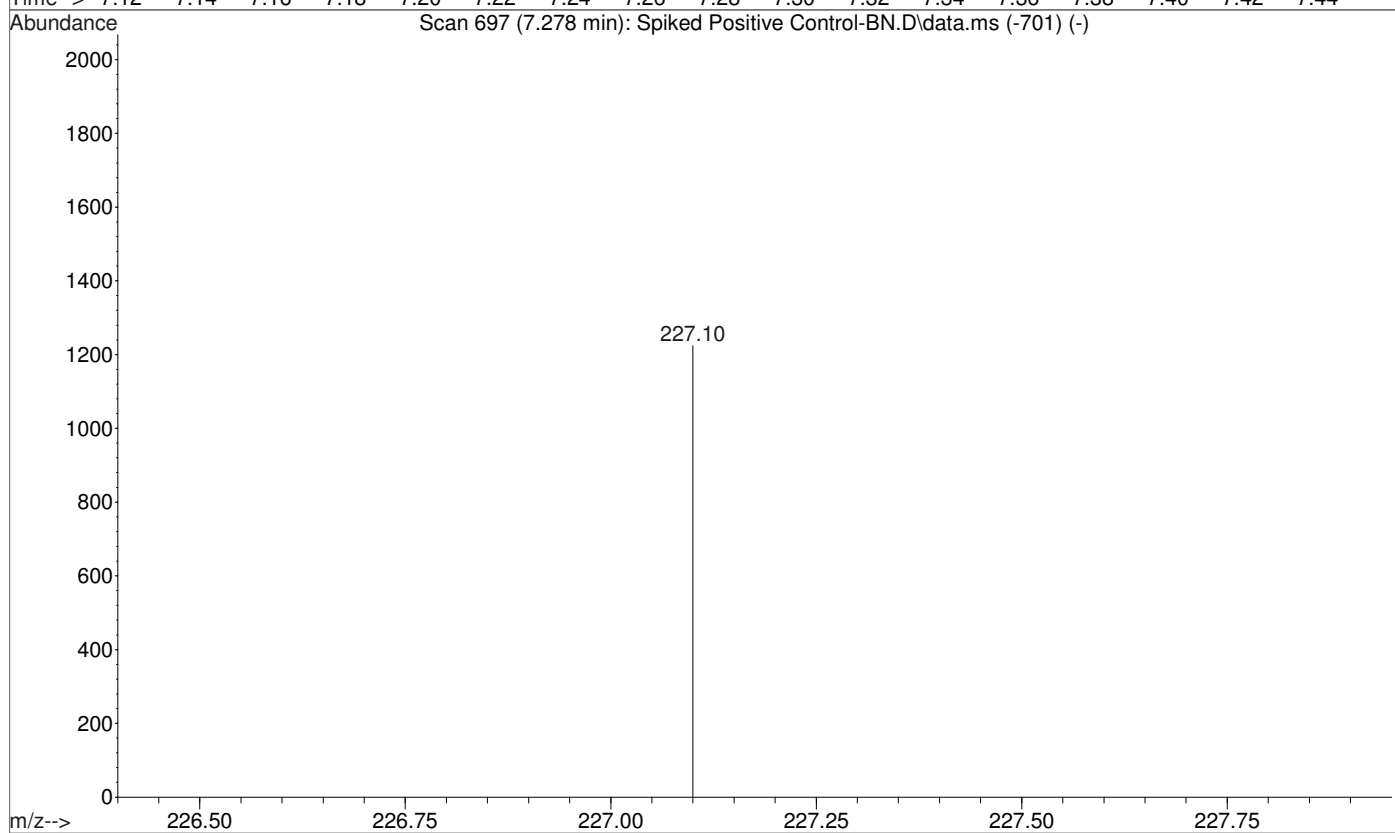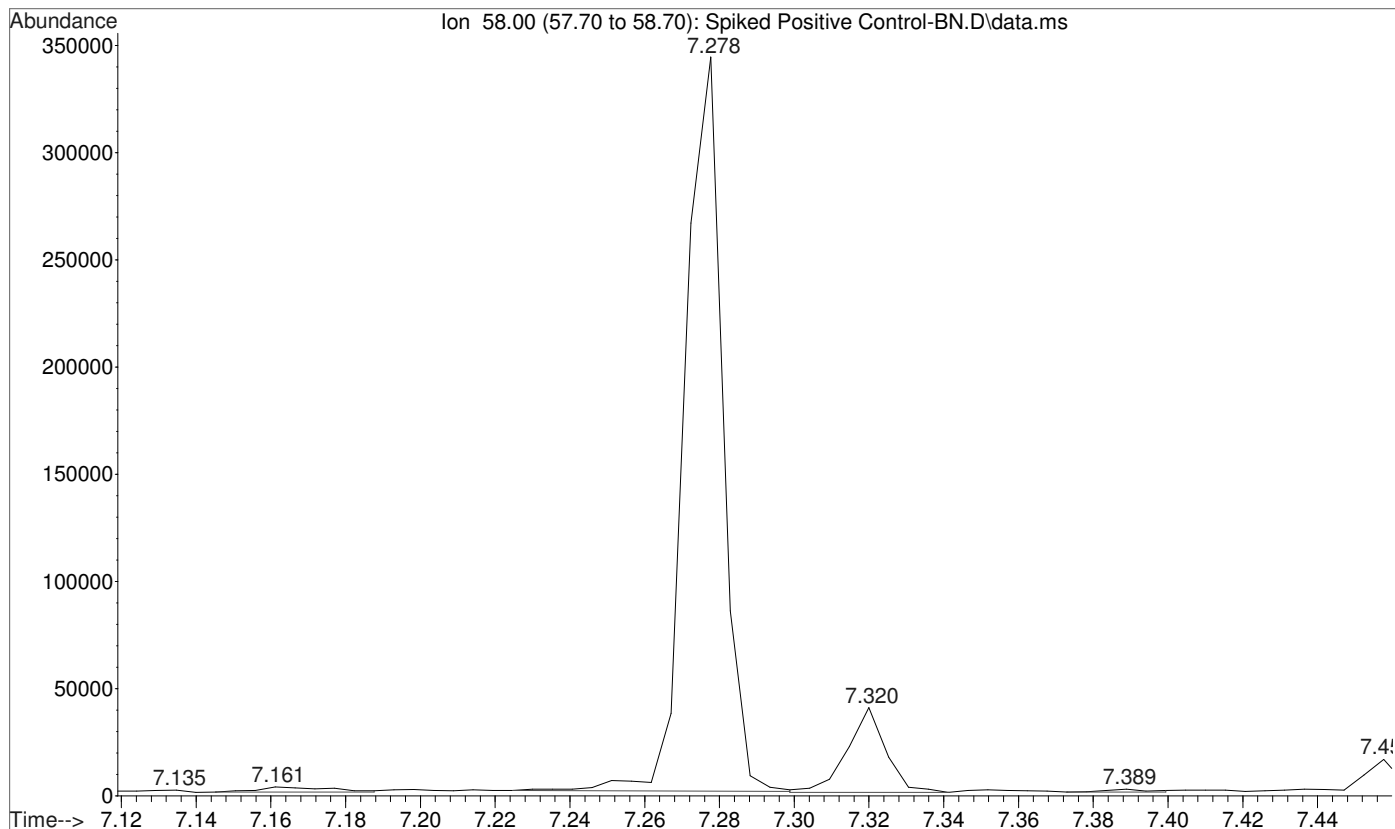



File :C:\gcms\1\data\Blood\100215\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 03 Oct 2015 00:41 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

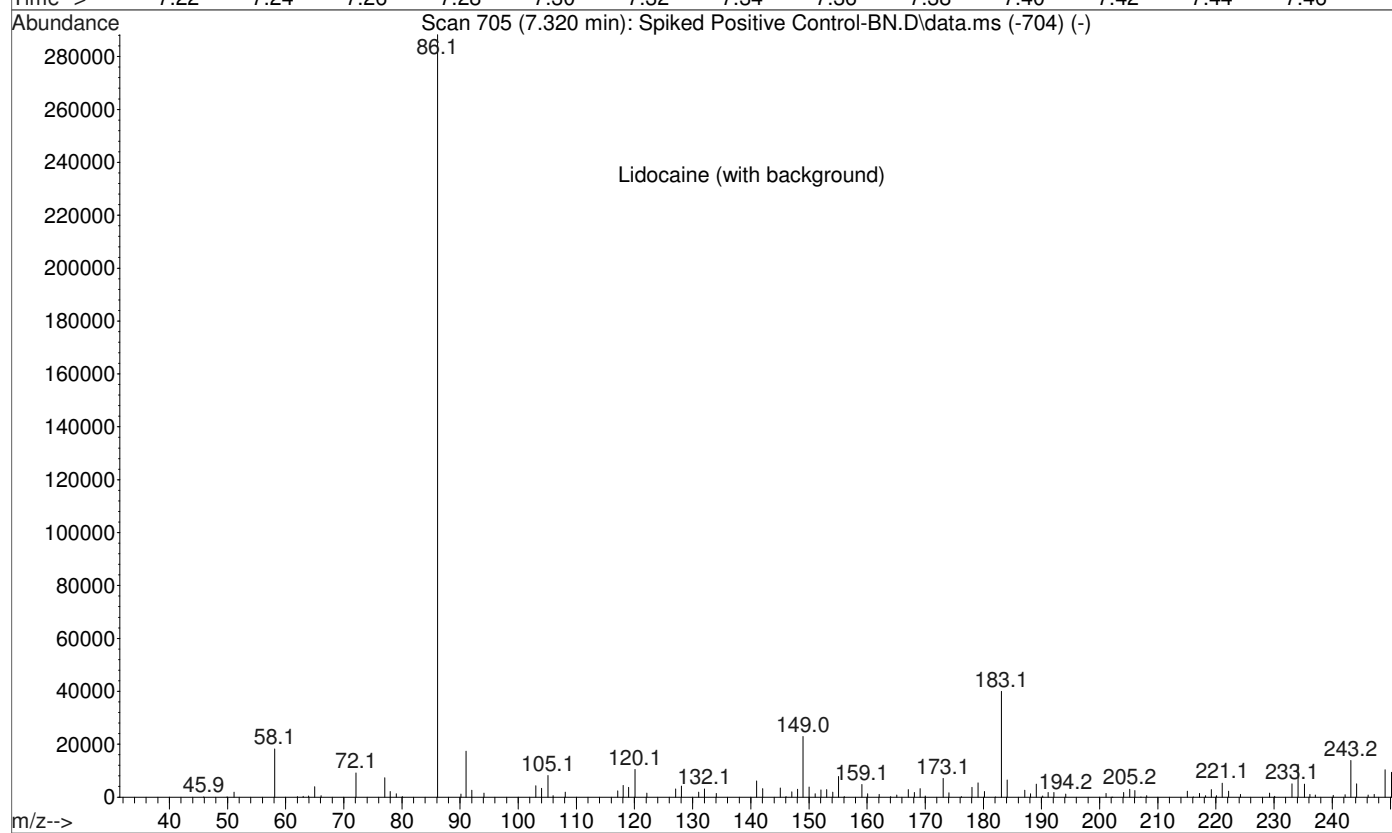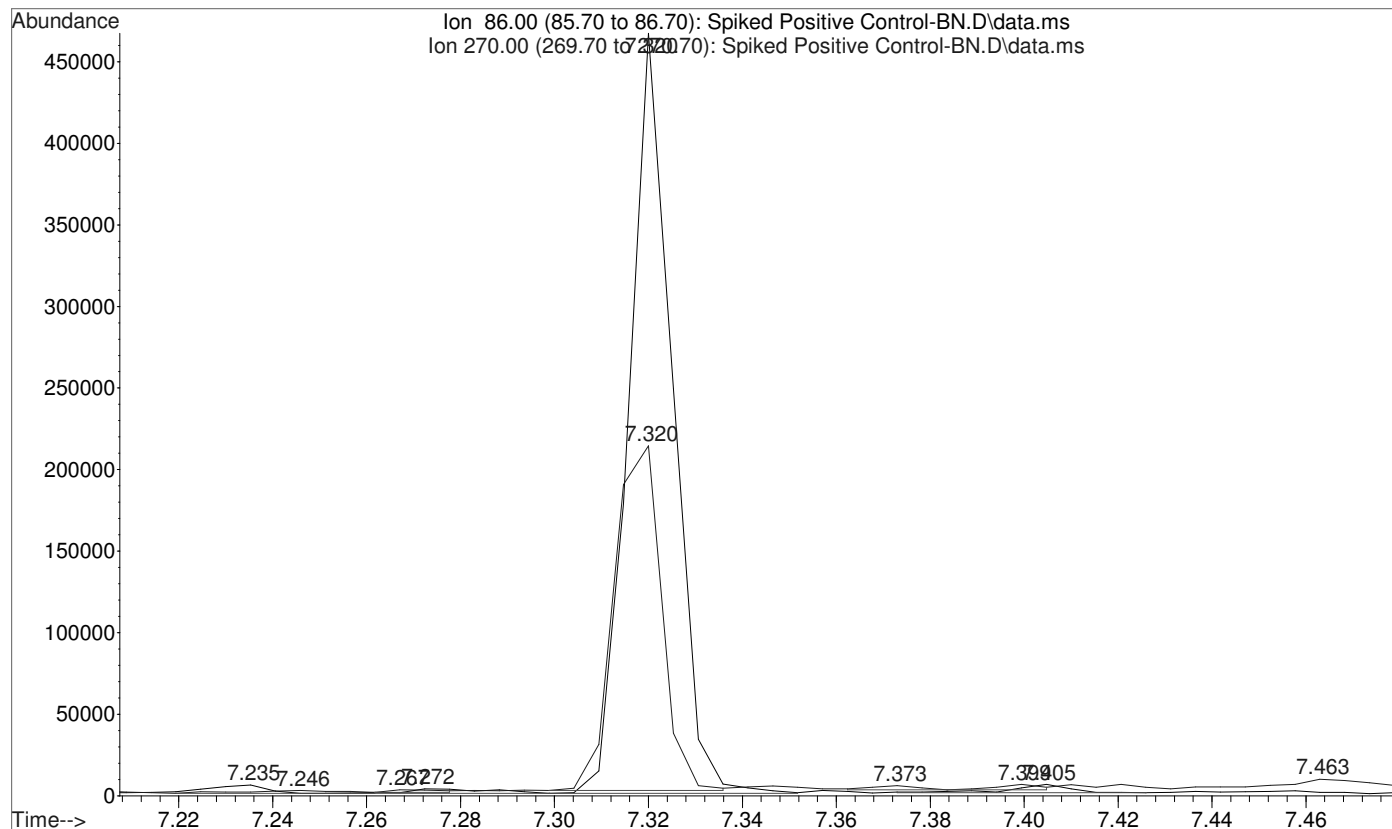



File :C:\gcms\1\data\Blood\100215\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 03 Oct 2015 00:41 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

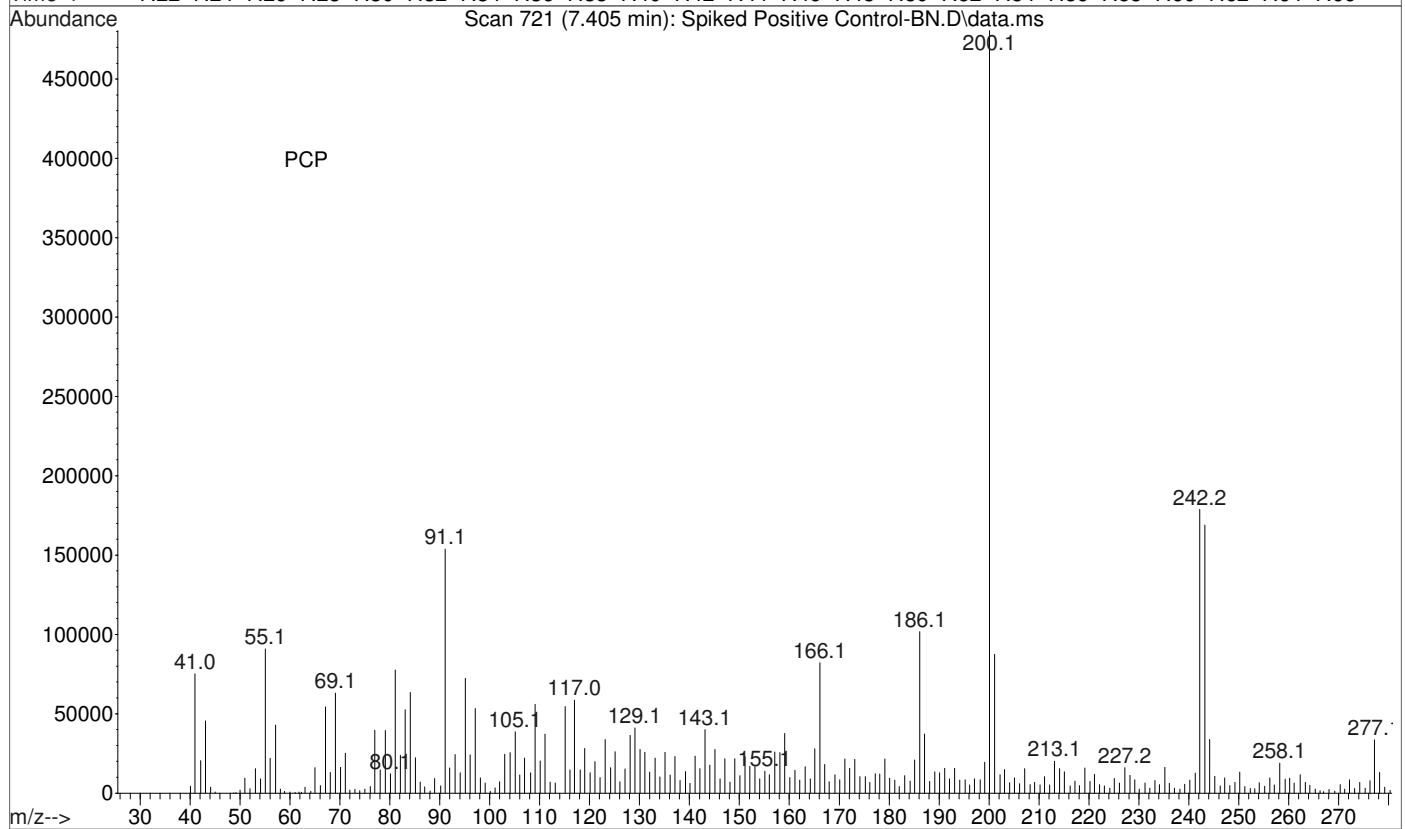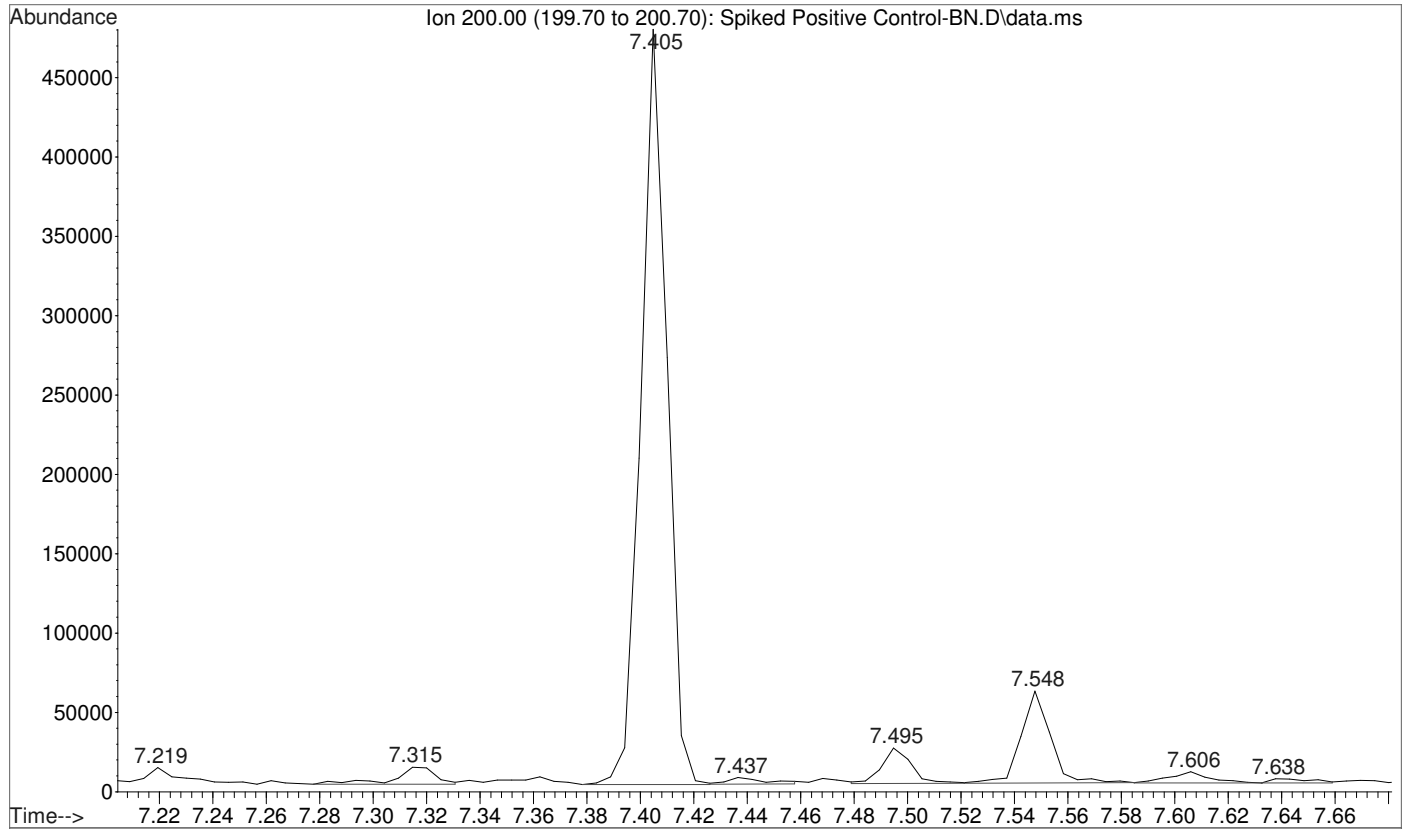



File :C:\gcms\1\data\Blood\100215\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 03 Oct 2015 00:41 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

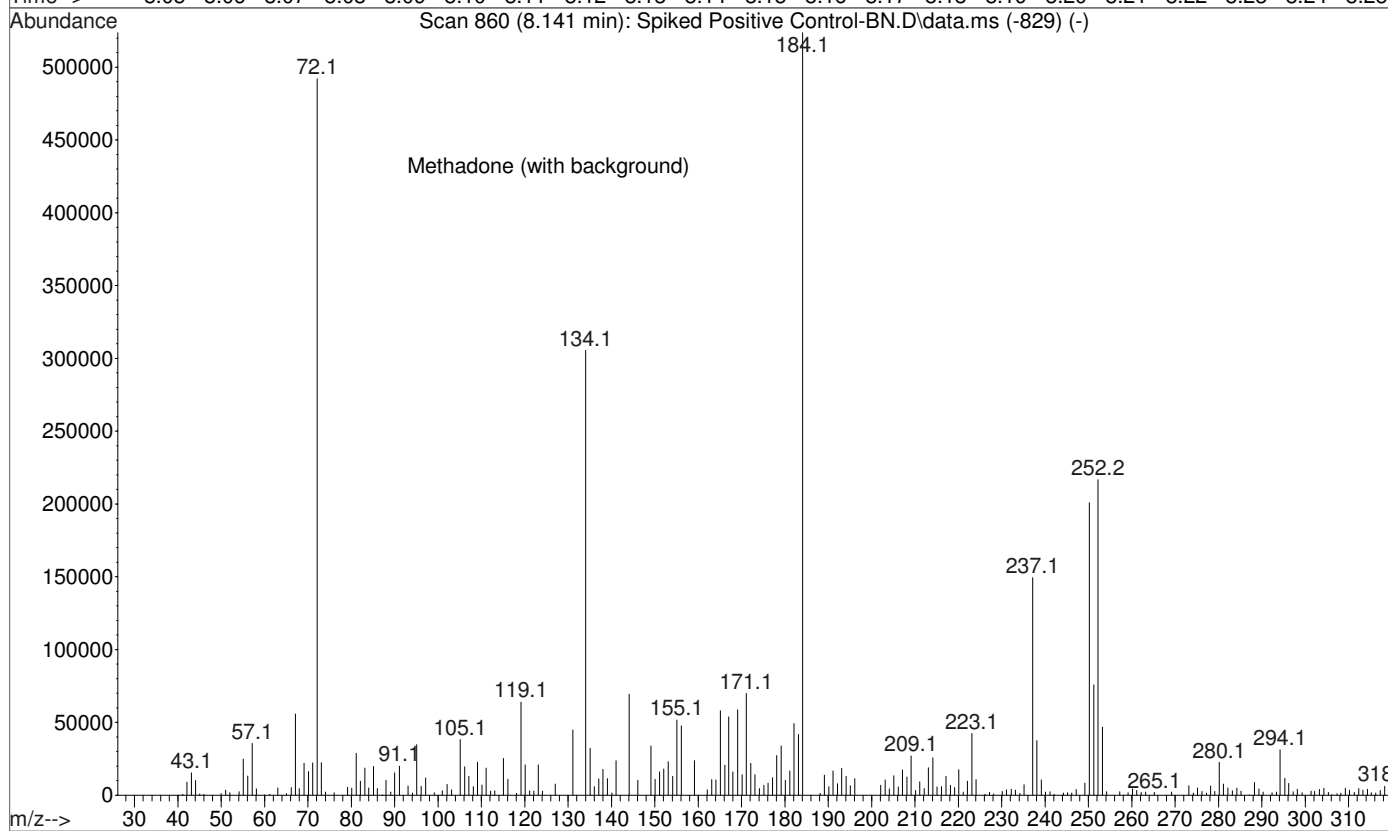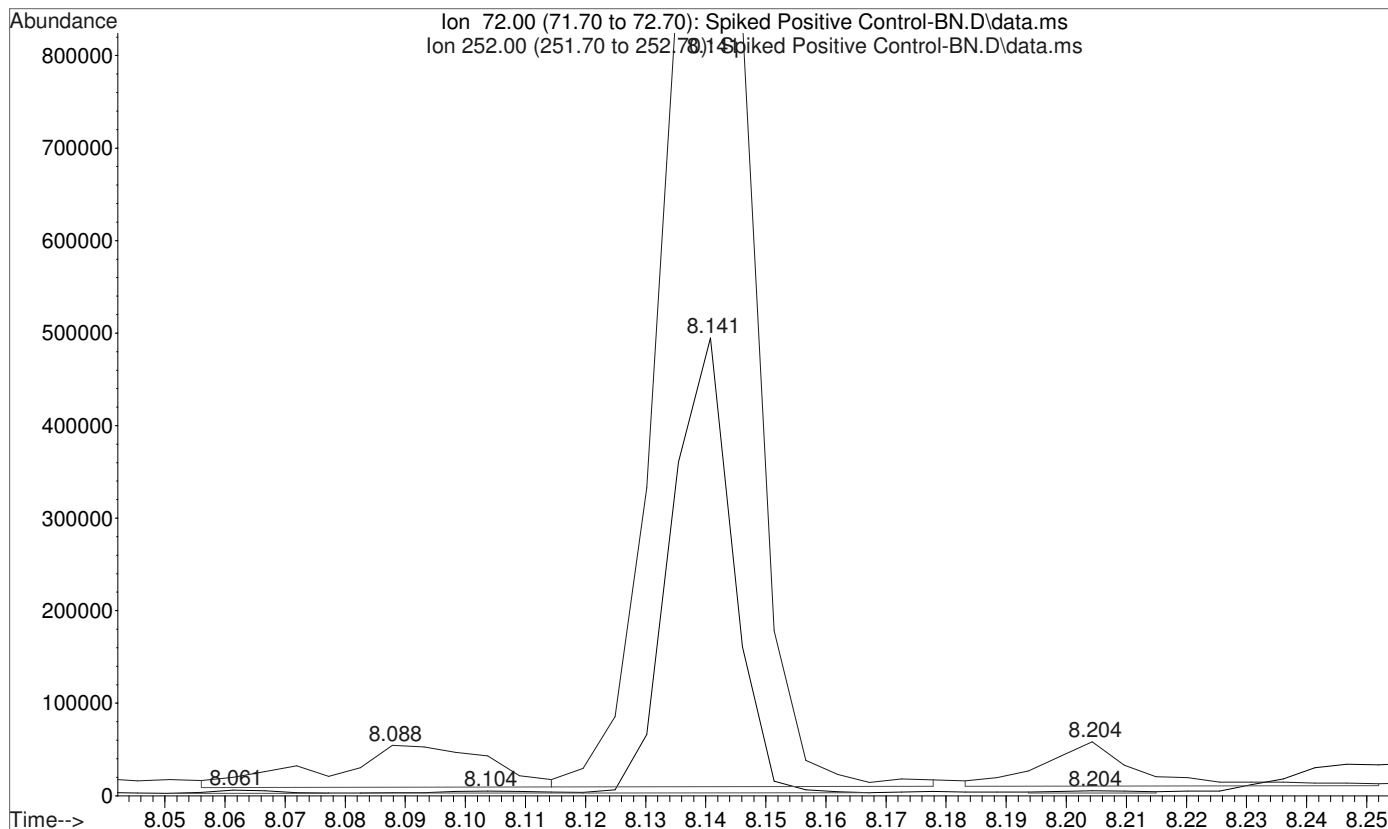



File :C:\gcms\1\data\Blood\100215\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 03 Oct 2015 00:41 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

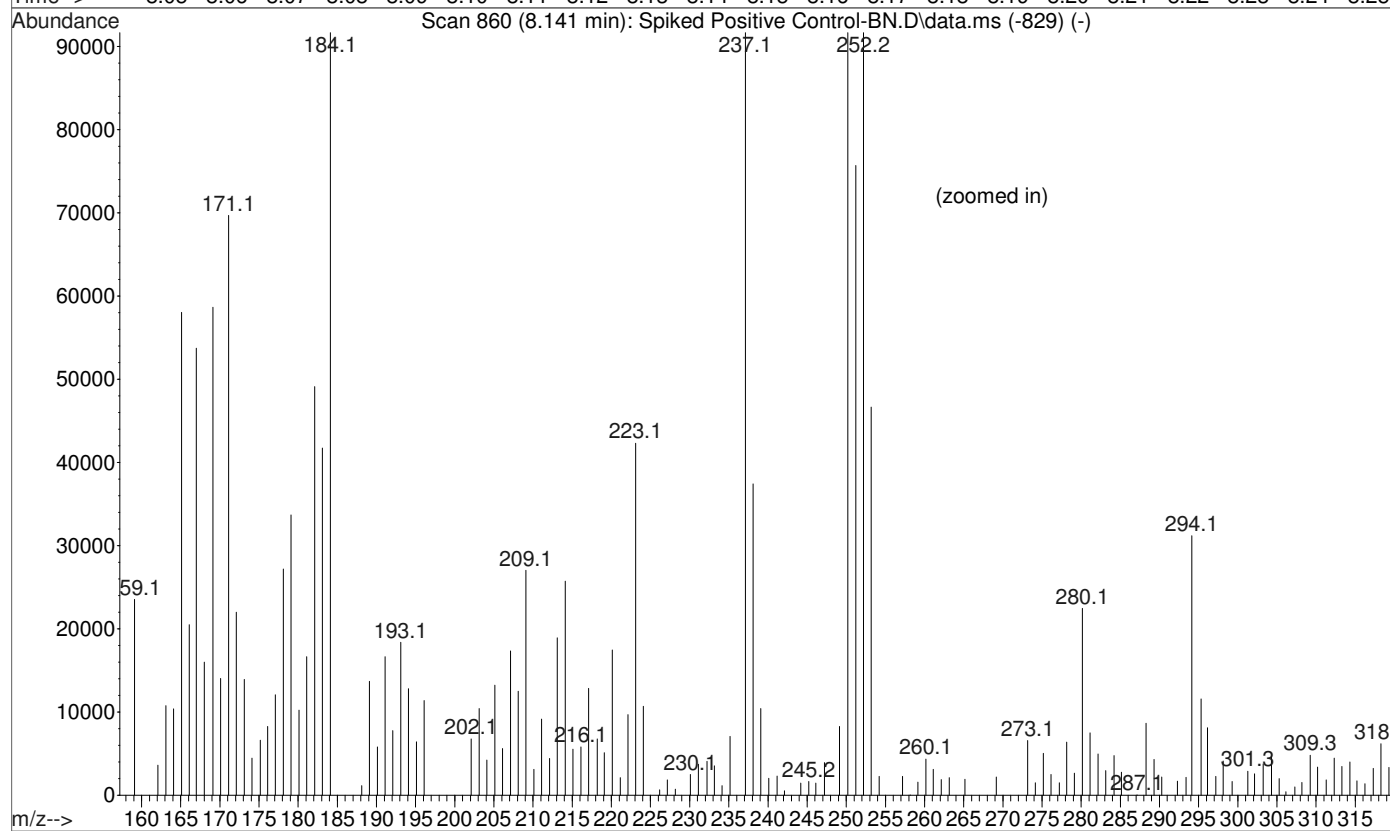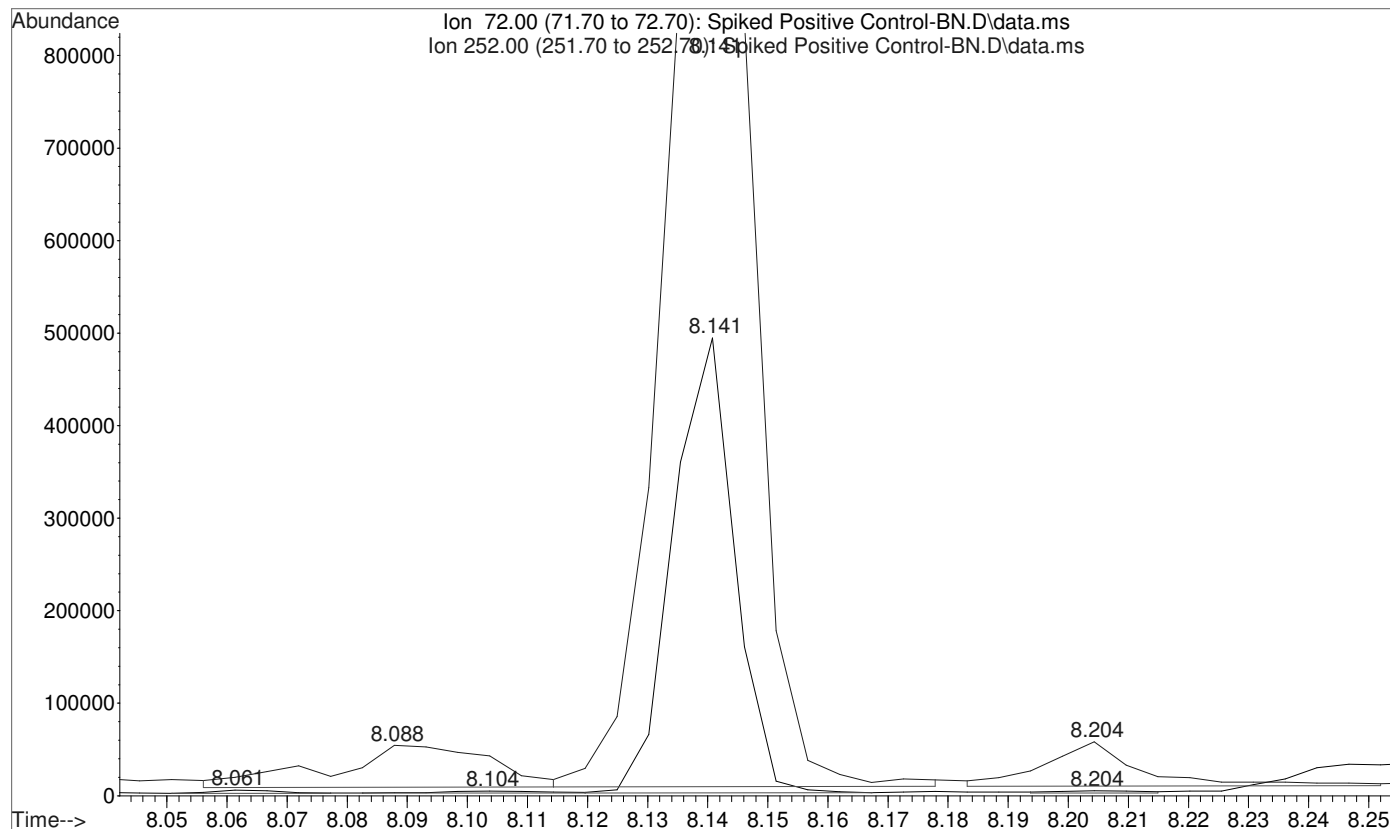



File :C:\gcms\1\data\Blood\100215\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 03 Oct 2015 00:41 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

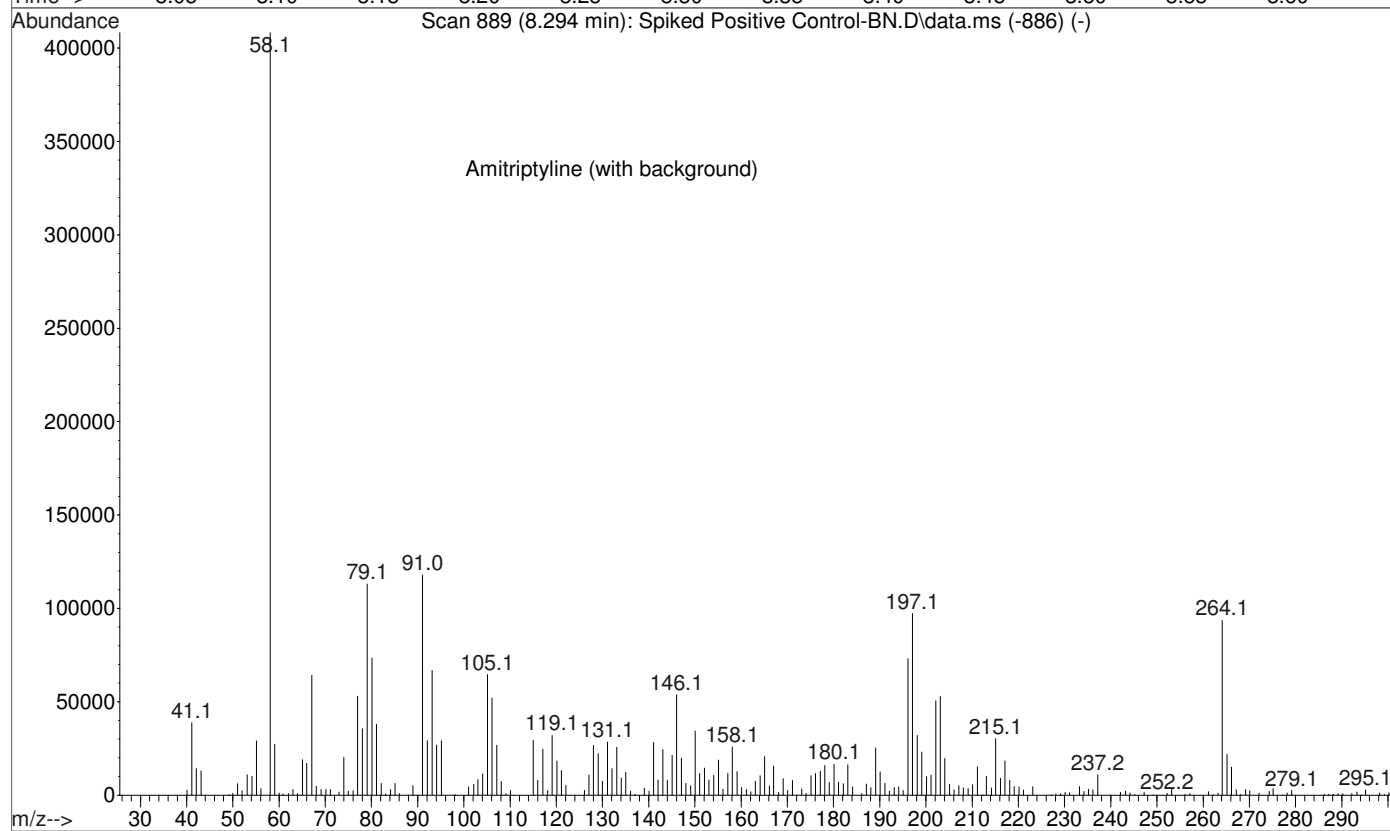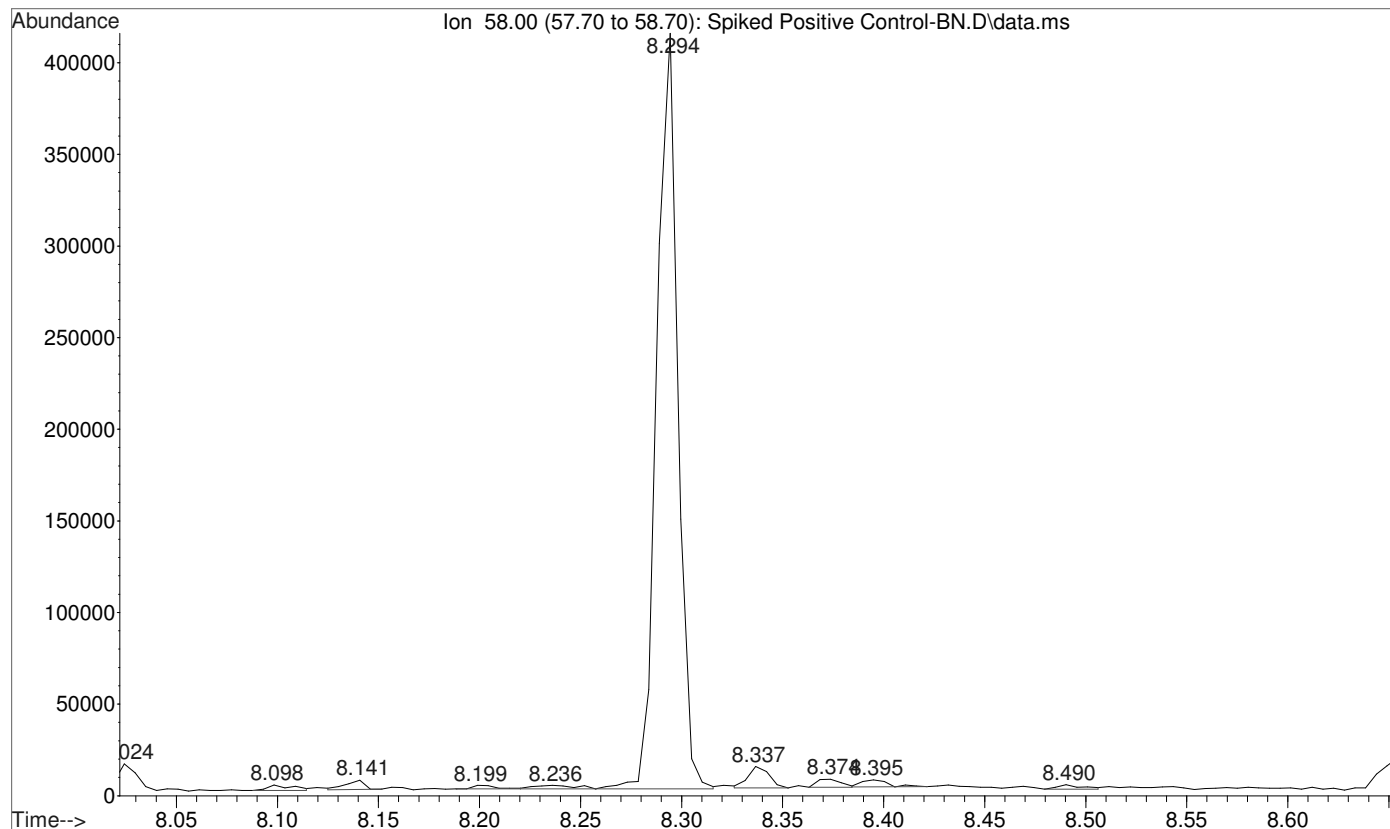



File :C:\gcms\1\data\Blood\100215\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 03 Oct 2015 00:41 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

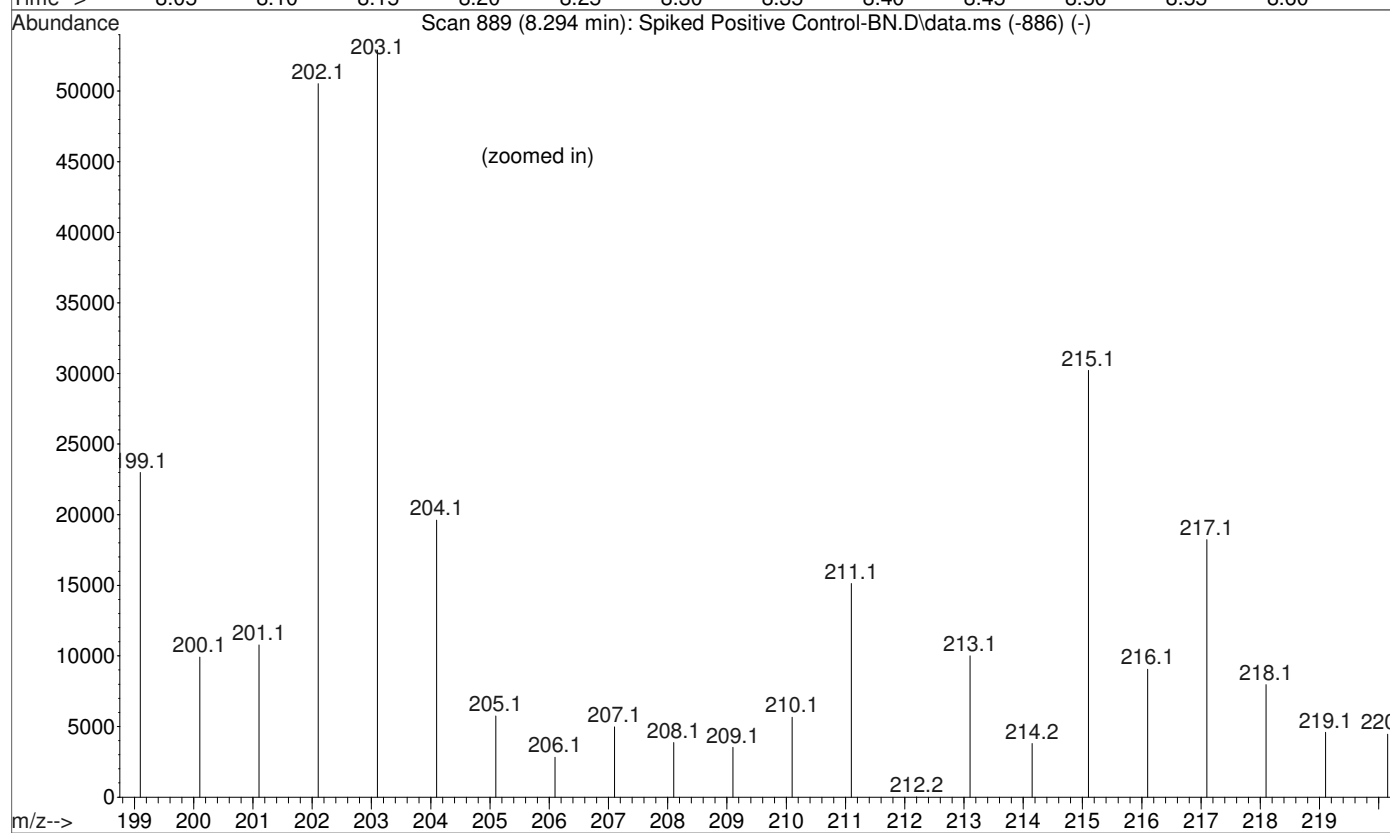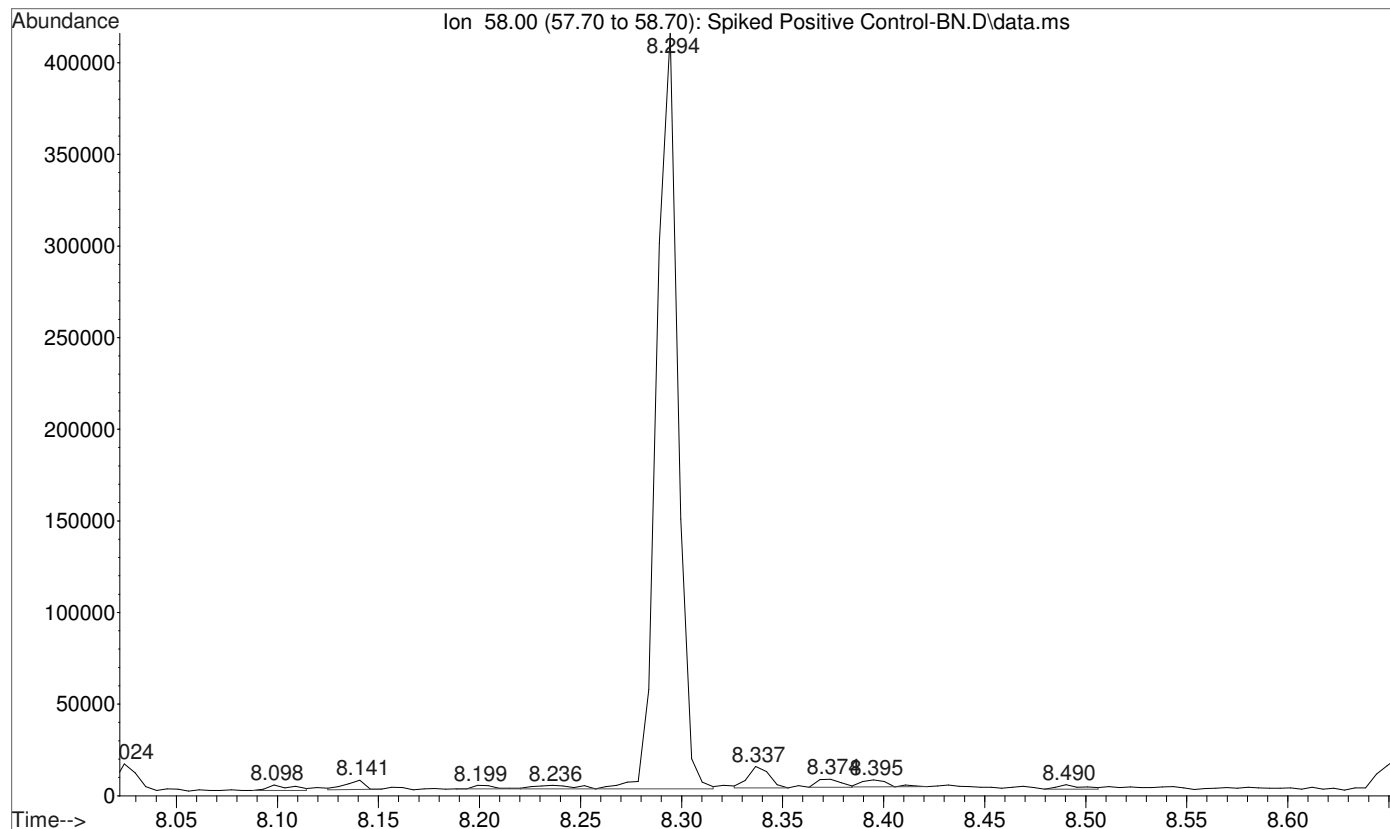



File :C:\gcms\1\data\Blood\100215\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 03 Oct 2015 00:41 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

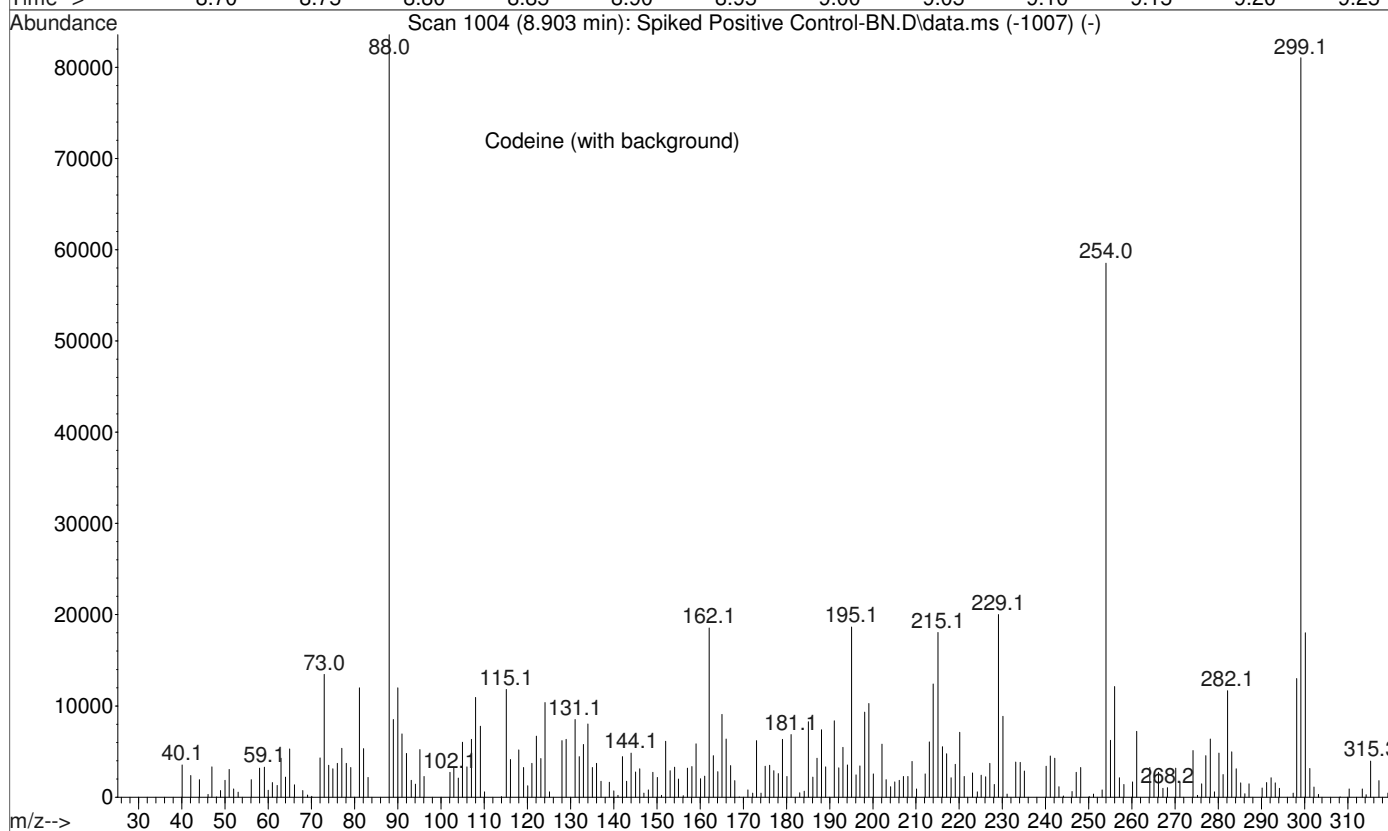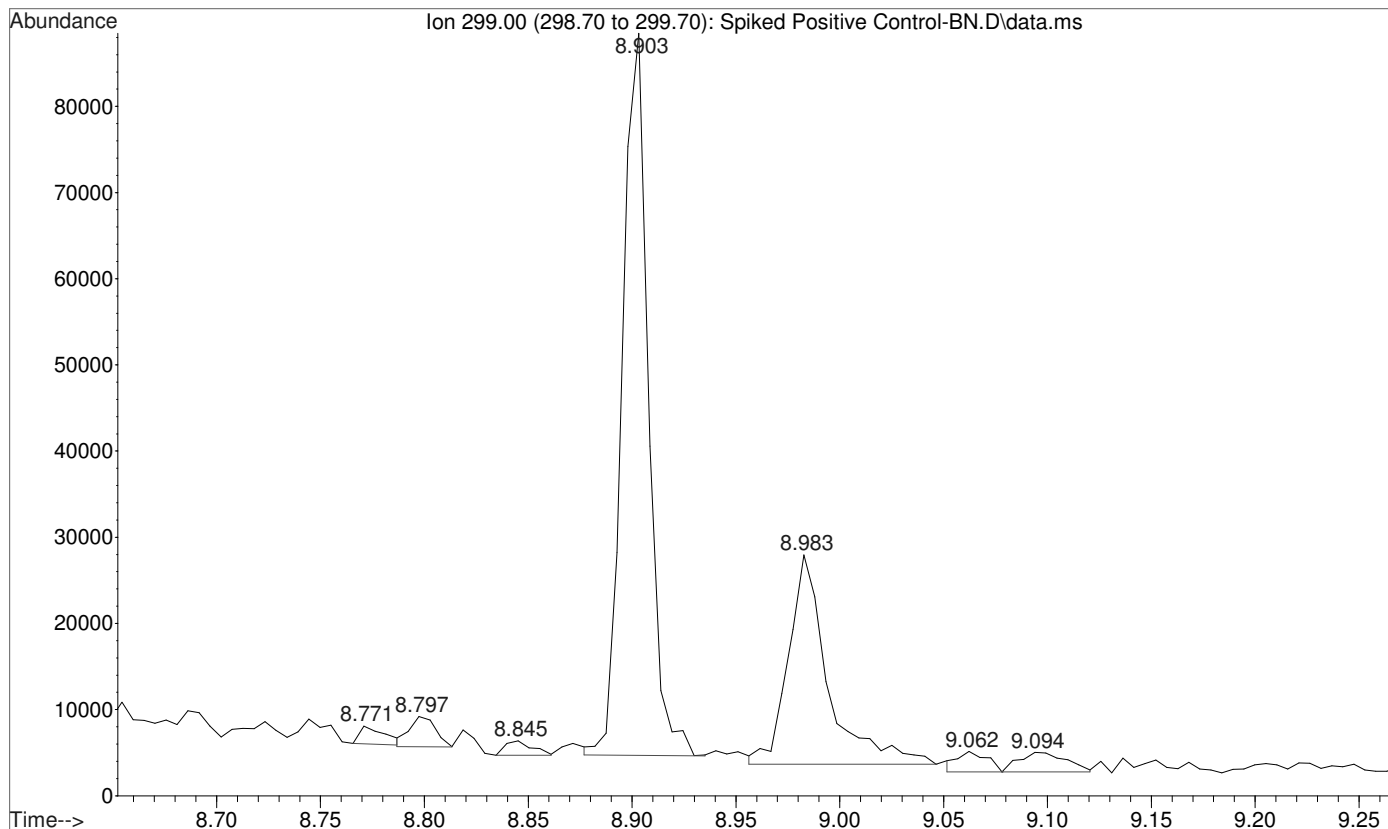

File :C:\gcms\1\data\Blood\100215\Spiked Positive Control-BN.D
Operator : ISP\datastor
Acquired : 03 Oct 2015 00:41 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1
Vial Number: 2

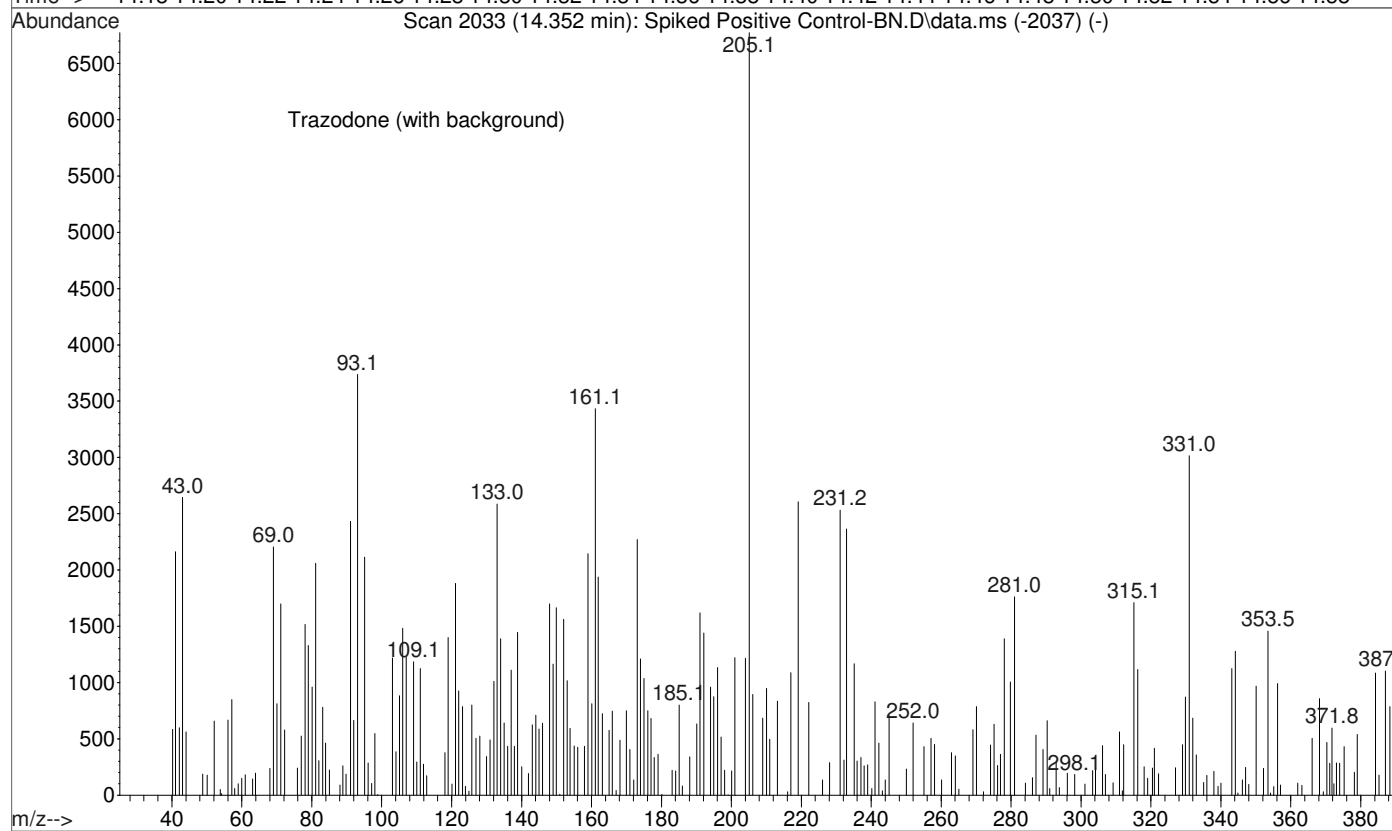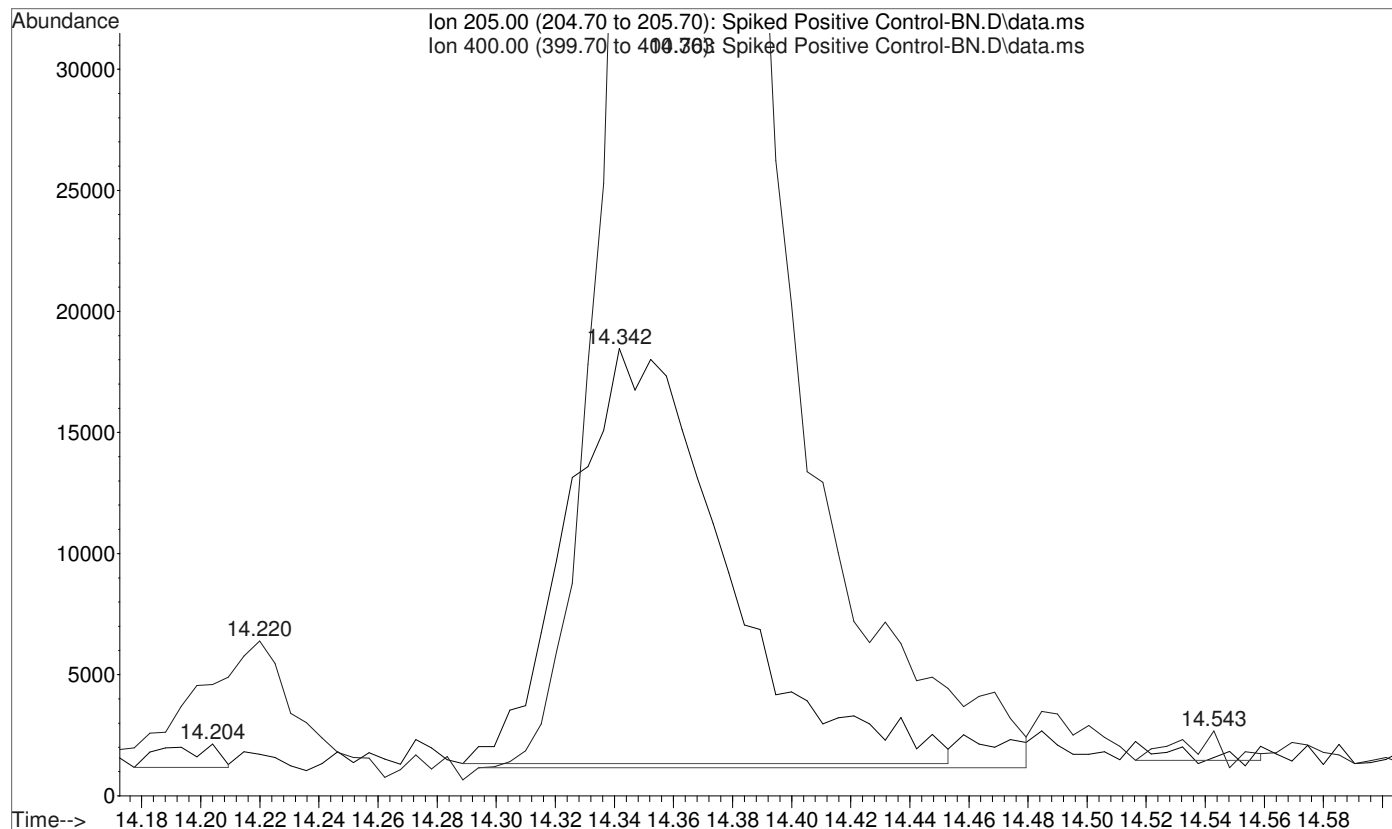

File :C:\gcms\1\data\Blood\100215\prbLK2.D
Operator : ISP\datastor
Acquired : 03 Oct 2015 01:04 using AcqMethod BNSB120510.M
Instrument : Major Mass Spec
Sample Name: Solvent Blank
Misc Info : Chloroform
Vial Number: 99

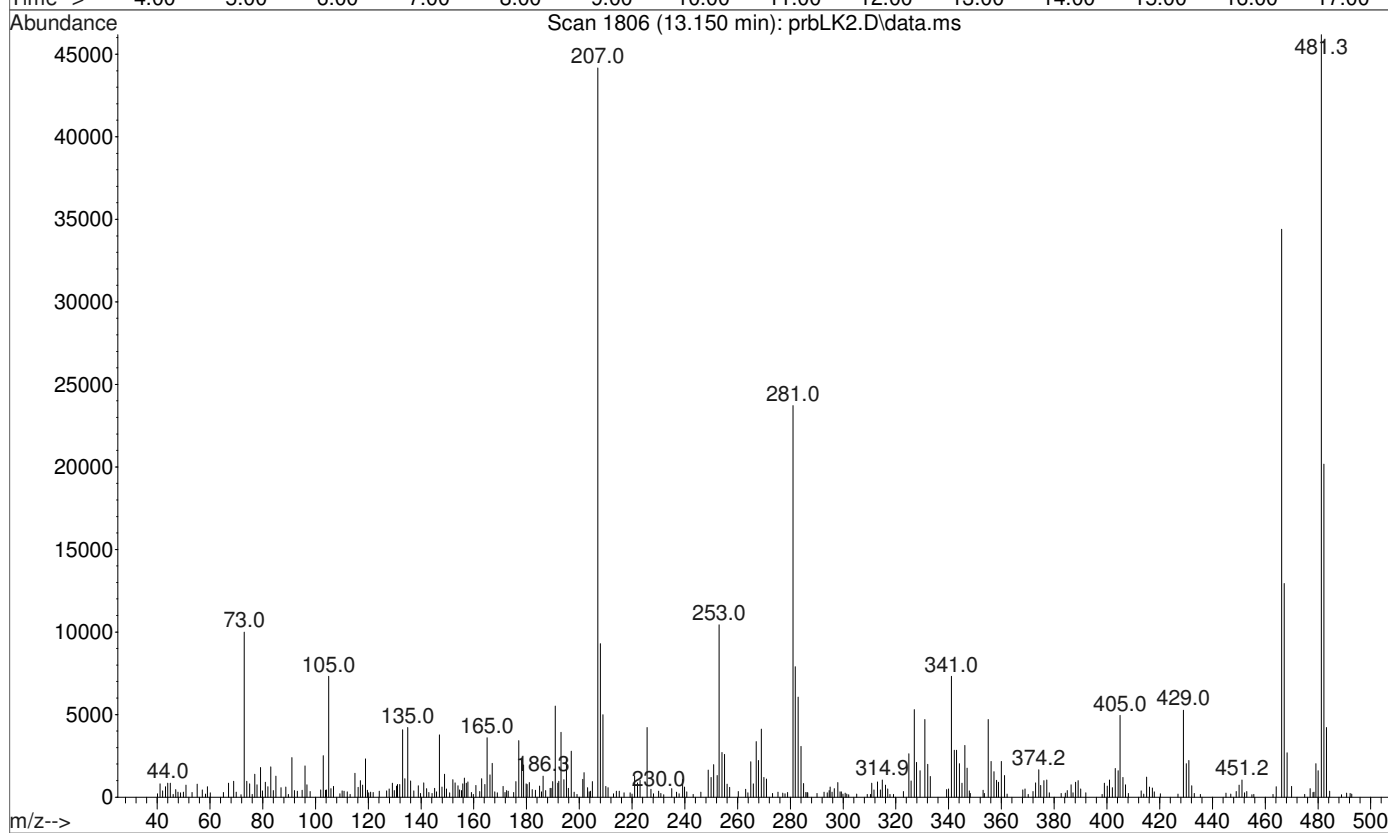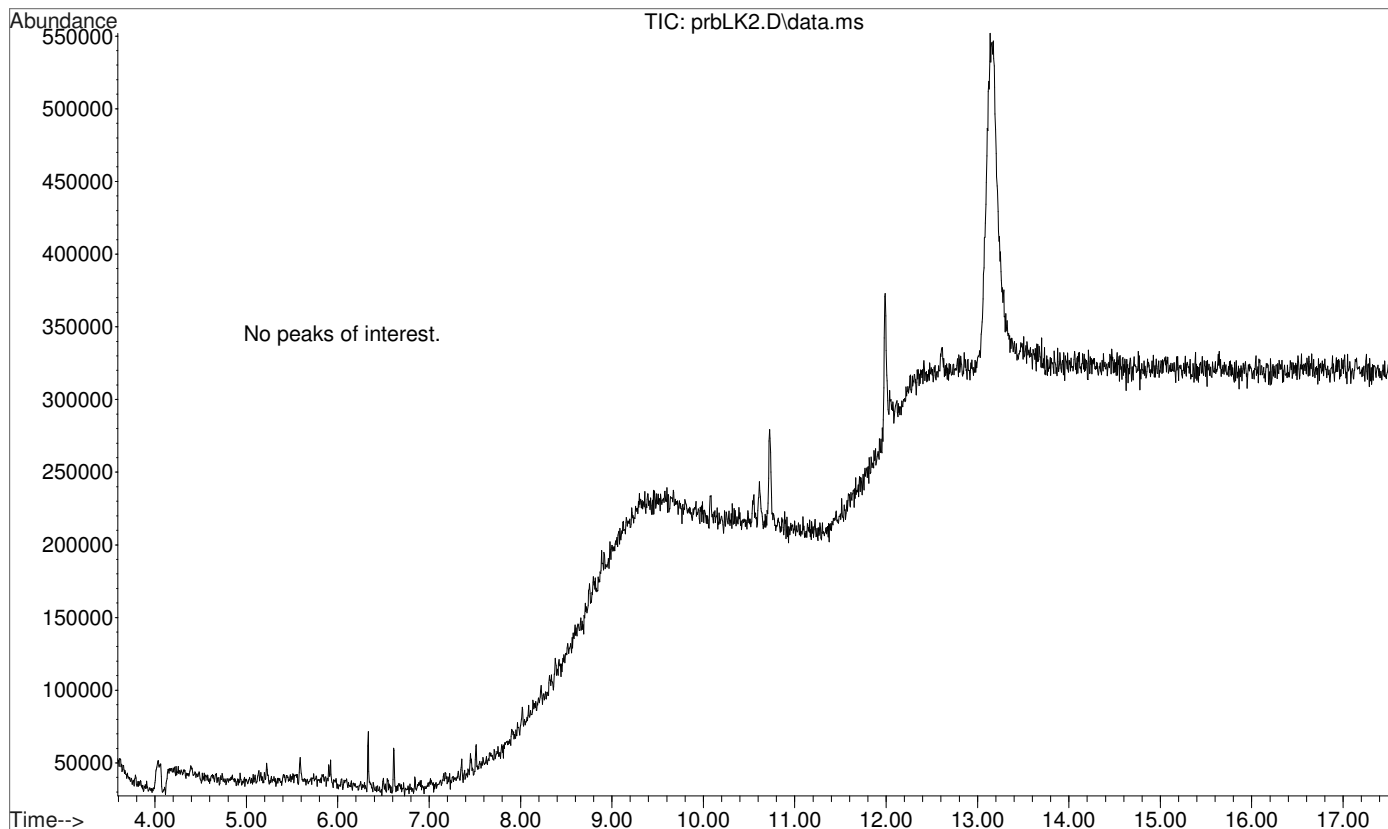

Analytical Method 3.6.1 & 3.6.7 QA Check List

Run Start Date: 10/02/15

Analyst: DND

(Long GC/MS temperature program)



Positive Control Compound List



- Phentermine (Cerilliant 30714-57F)
- Methamphetamine
- Nicotine
- Meperidine
- Caffeine
- Diphenhydramine
- Lidocaine
- PCP
- Methadone
- Amitriptyline
- Codeine
- Trazodone


Internal Standards

- Benzphetamine
- Papaverine


Optional back extraction **not** performed.
Samples reconstituted in methanol.

File :C:\gcms\1\data\Blood\100215\Reinjection Longer GC Method\Pre
... run Solvent Blankr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 03 Oct 2015 01:26 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Pre-run Solvent Blank
Misc Info : Chloroform

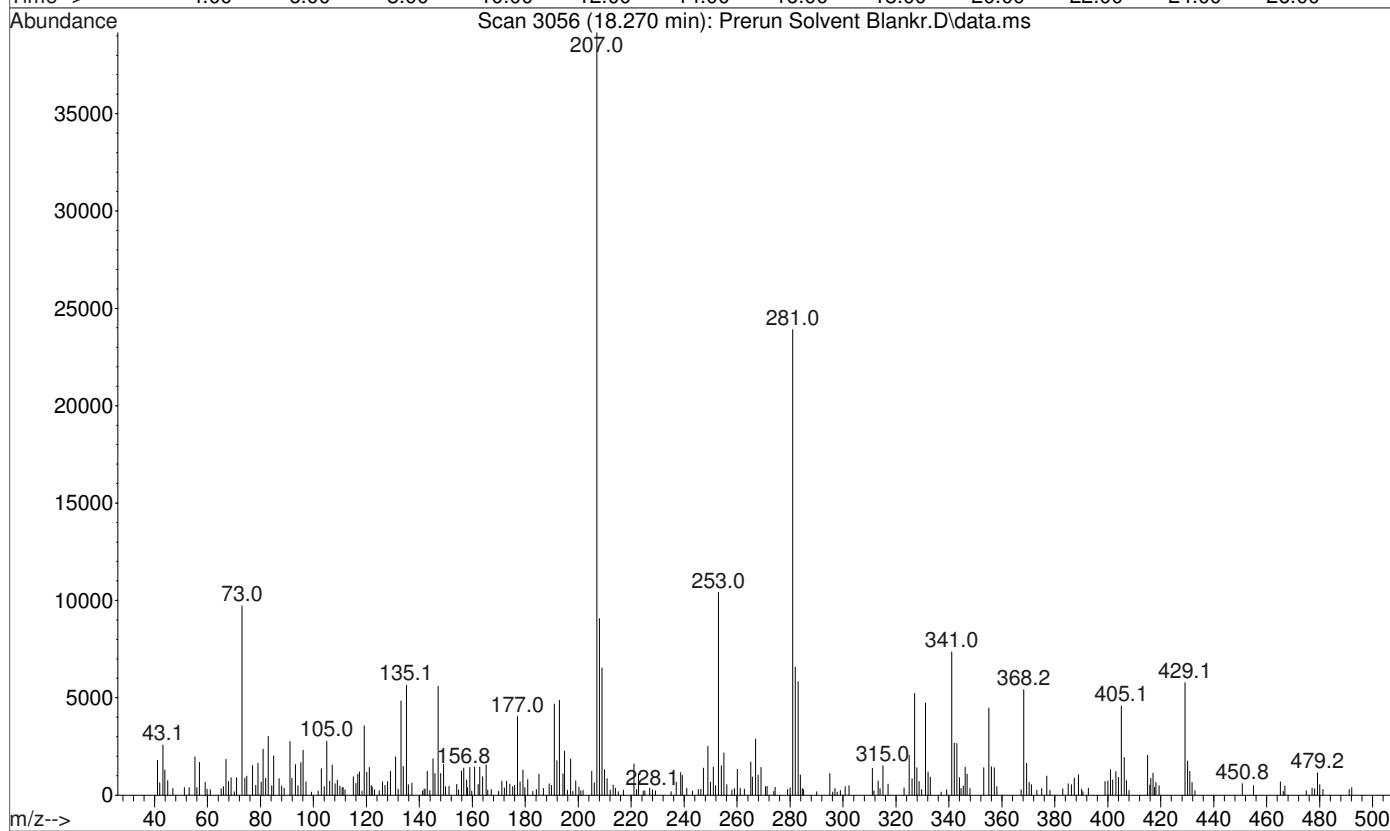
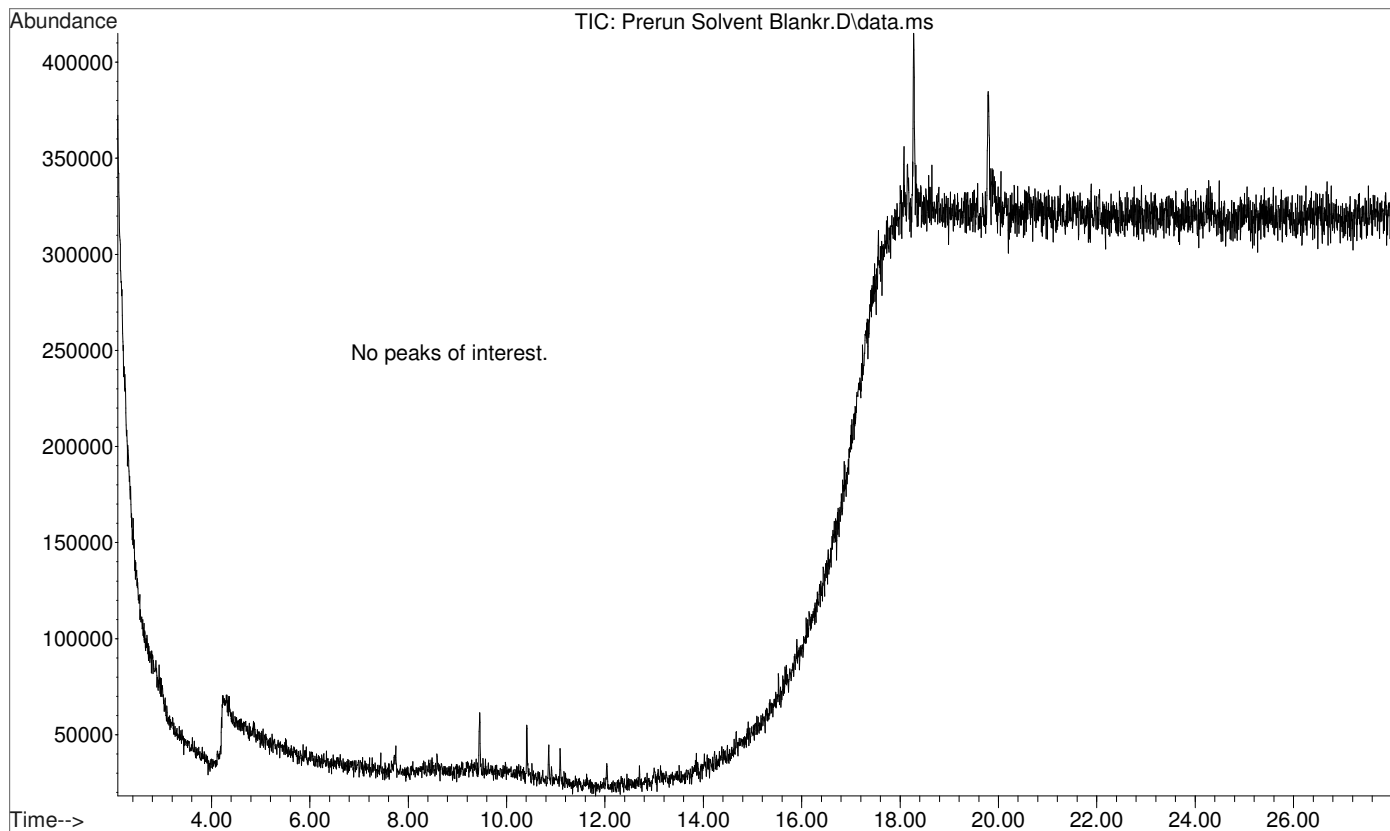






File :C:\gcms\1\data\Blood\100215\Reinjection Longer GC Method\Neg
... ative Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 03 Oct 2015 02:00 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1

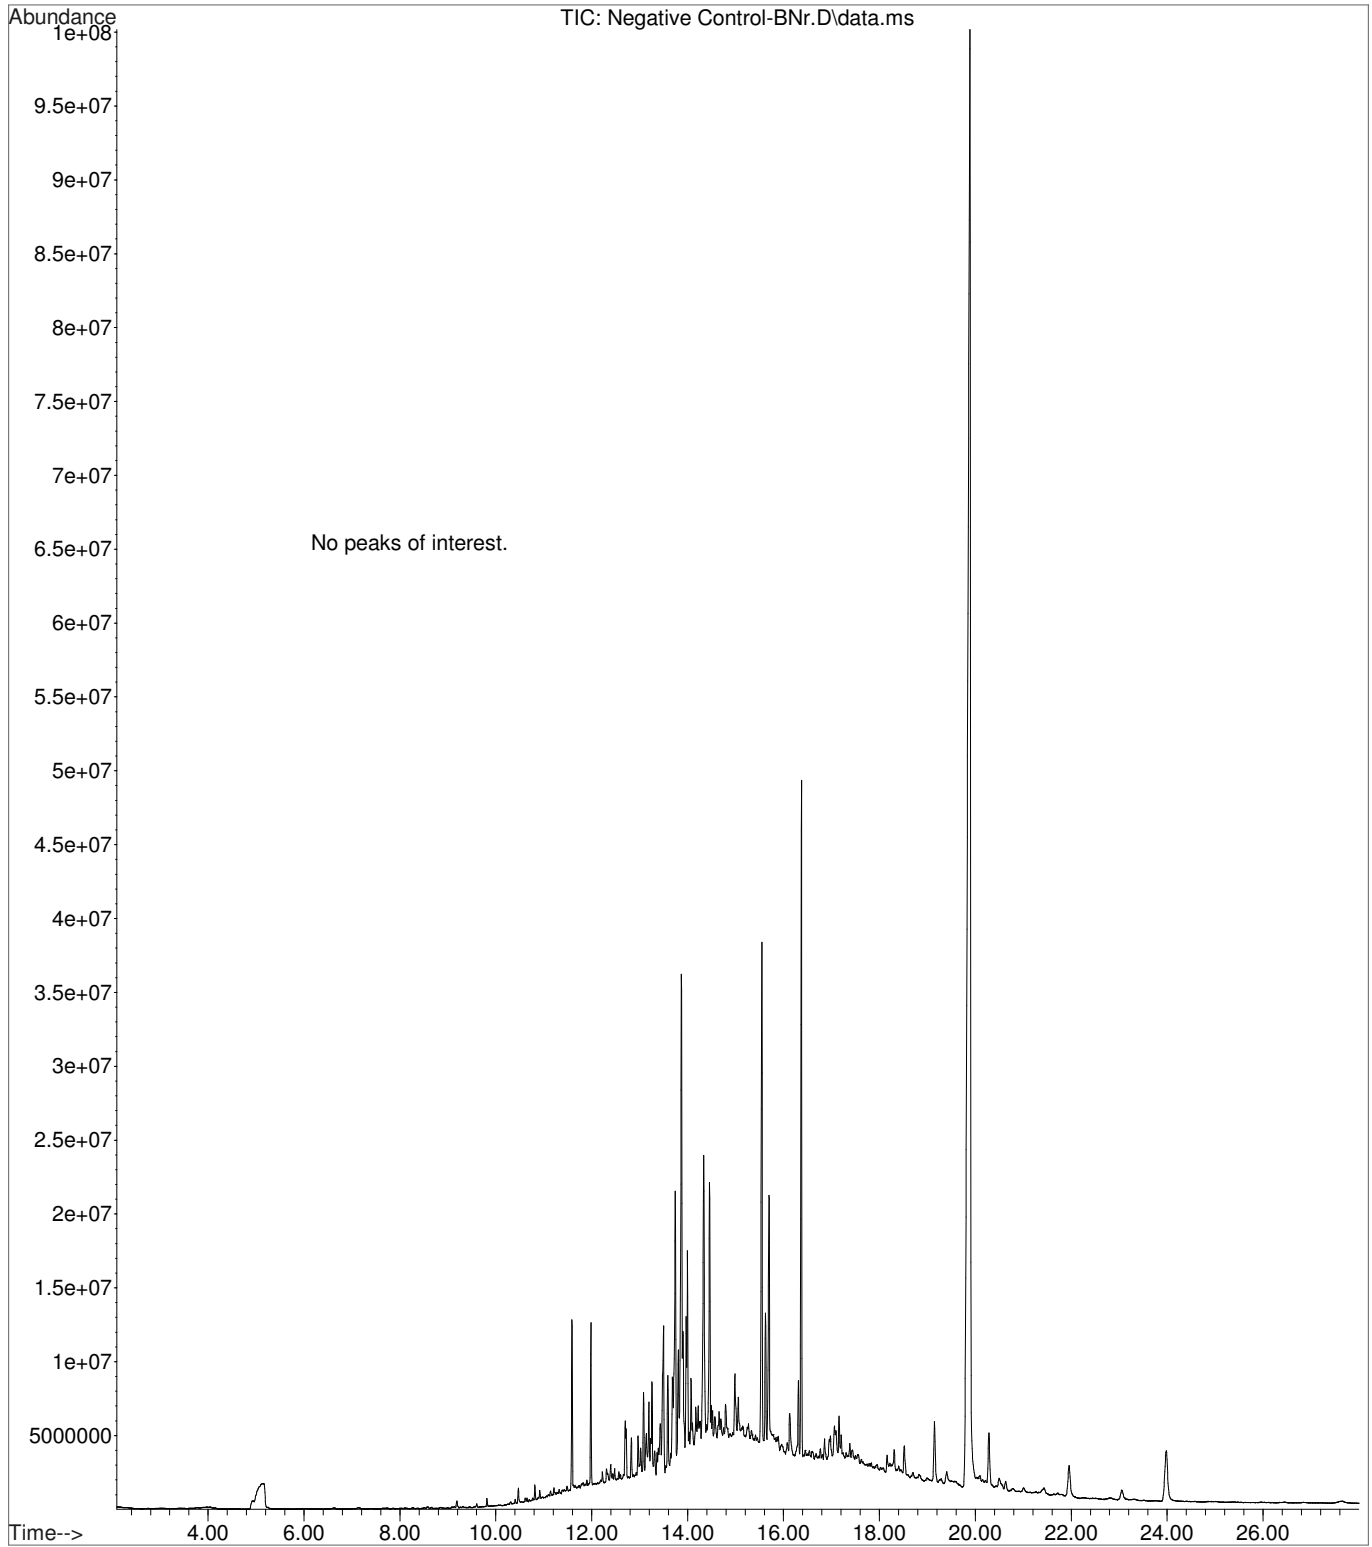

File :C:\gcms\1\data\Blood\100215\Reinjection Longer GC Method\Neg
... ative Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 03 Oct 2015 02:00 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1

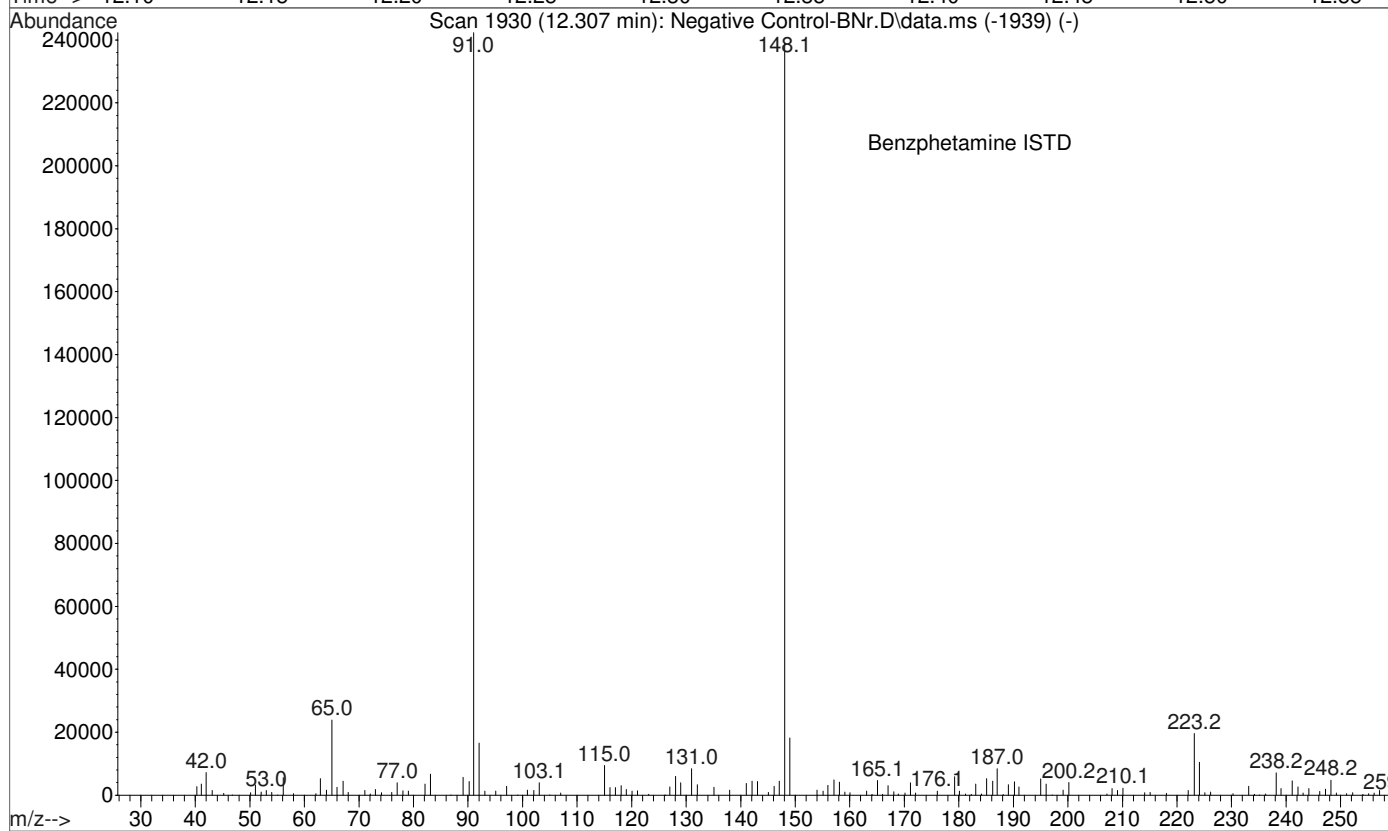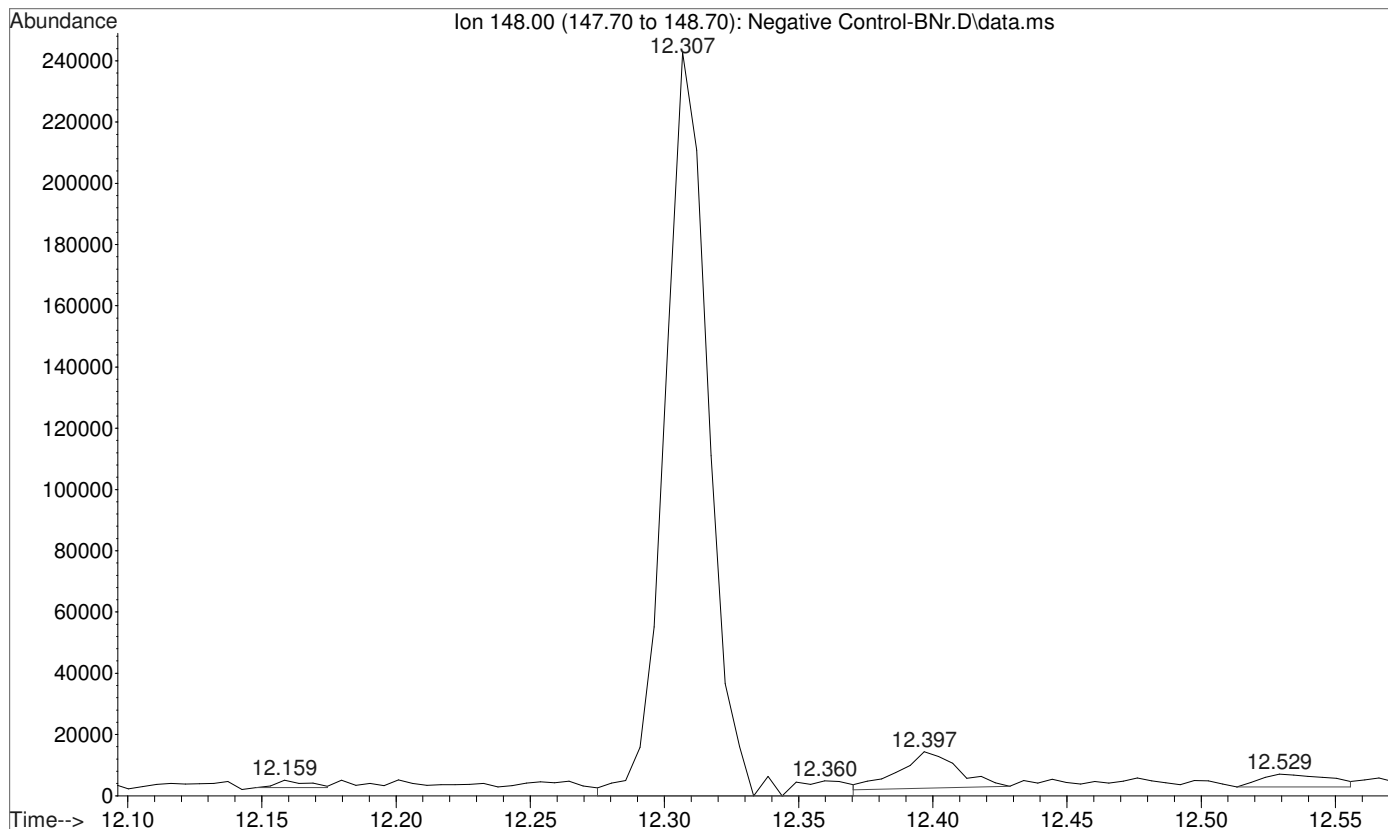


File :C:\gcms\1\data\Blood\100215\Reinjection Longer GC Method\Neg
... ative Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 03 Oct 2015 02:00 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Negative Control - Utak Lot B0689
Misc Info : Analytical Method 3.6.1

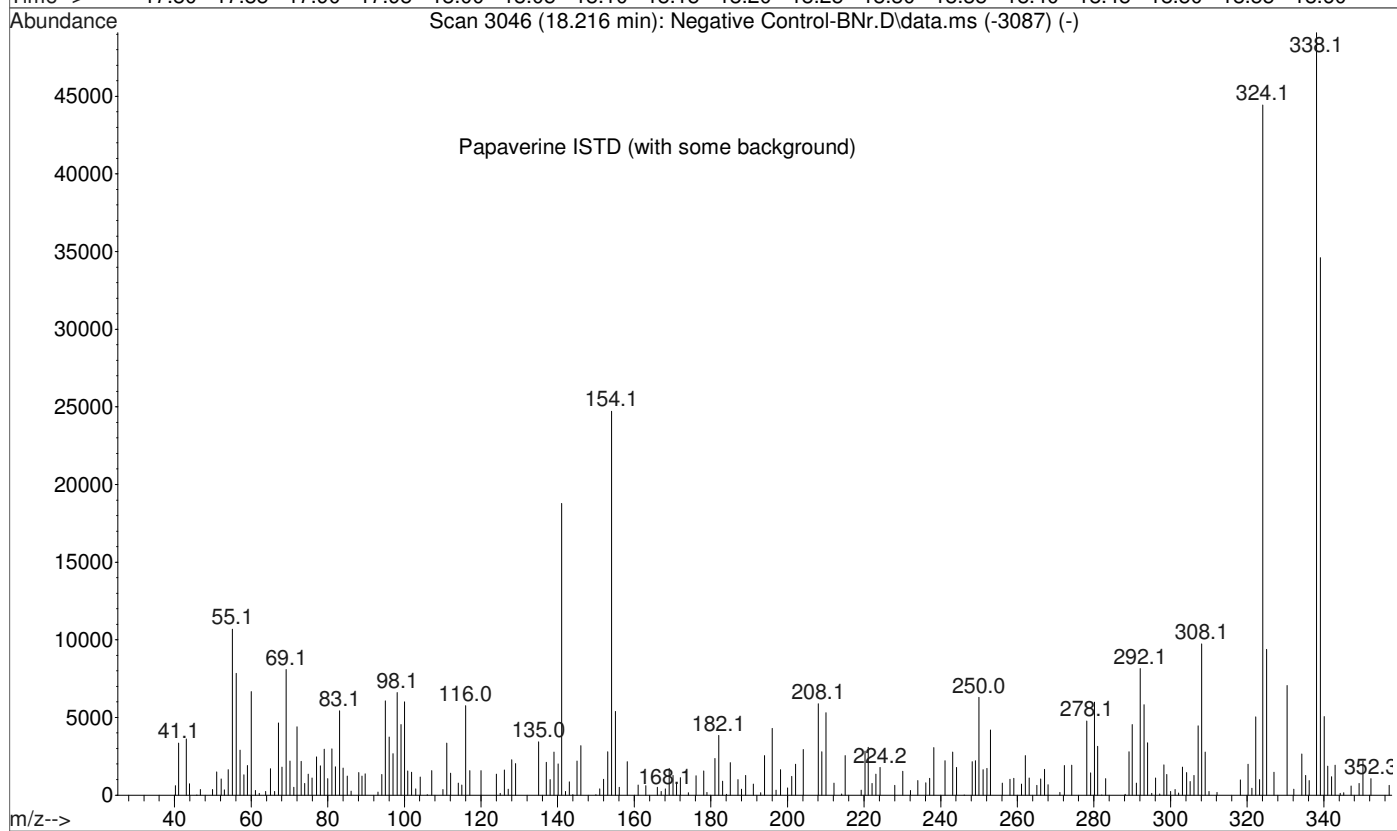
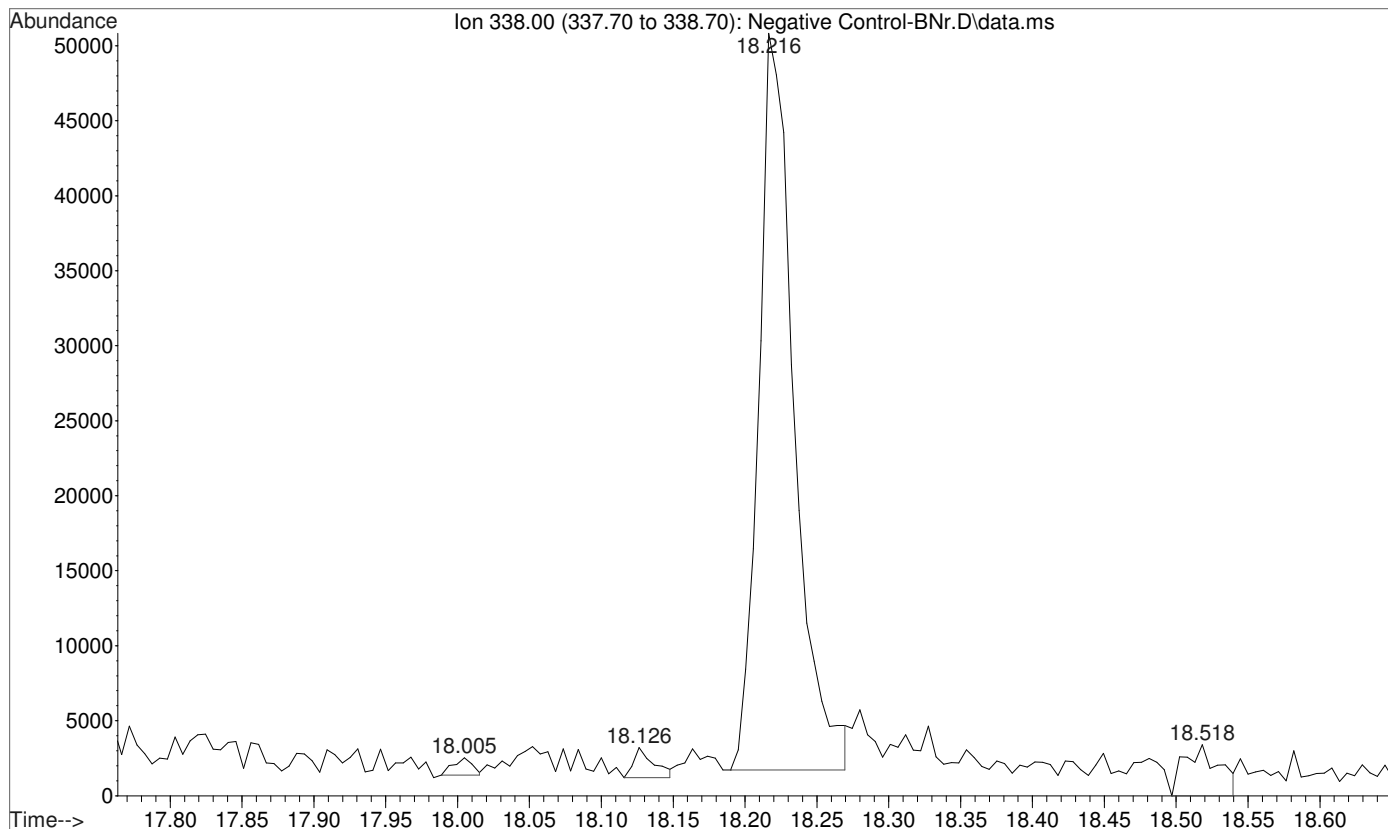






File :C:\gcms\1\data\Blood\100215\Reinjection Longer GC Method\Spi
... ked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 03 Oct 2015 02:34 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

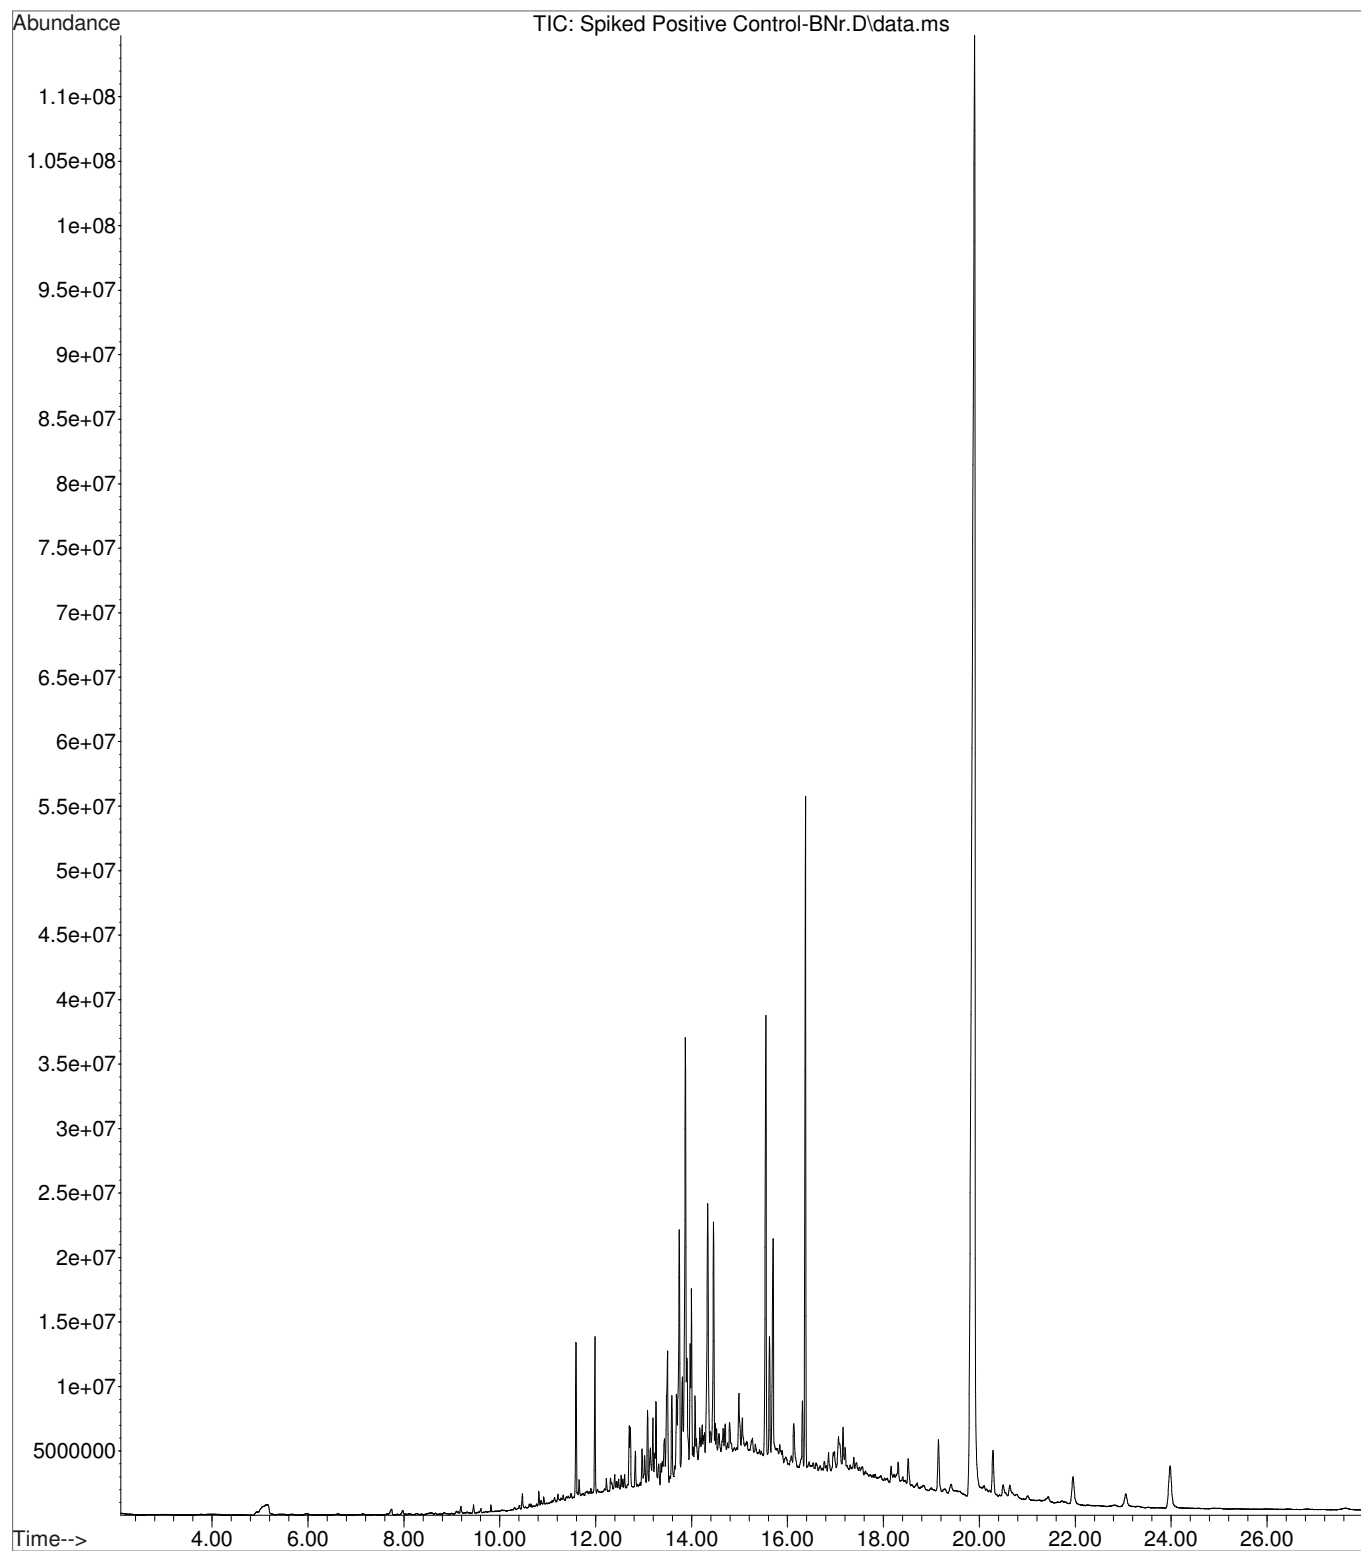



File :C:\gcms\1\data\Blood\100215\Reinjection Longer GC Method\Spiked Positive Control-BNr.D
...
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 03 Oct 2015 02:34 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

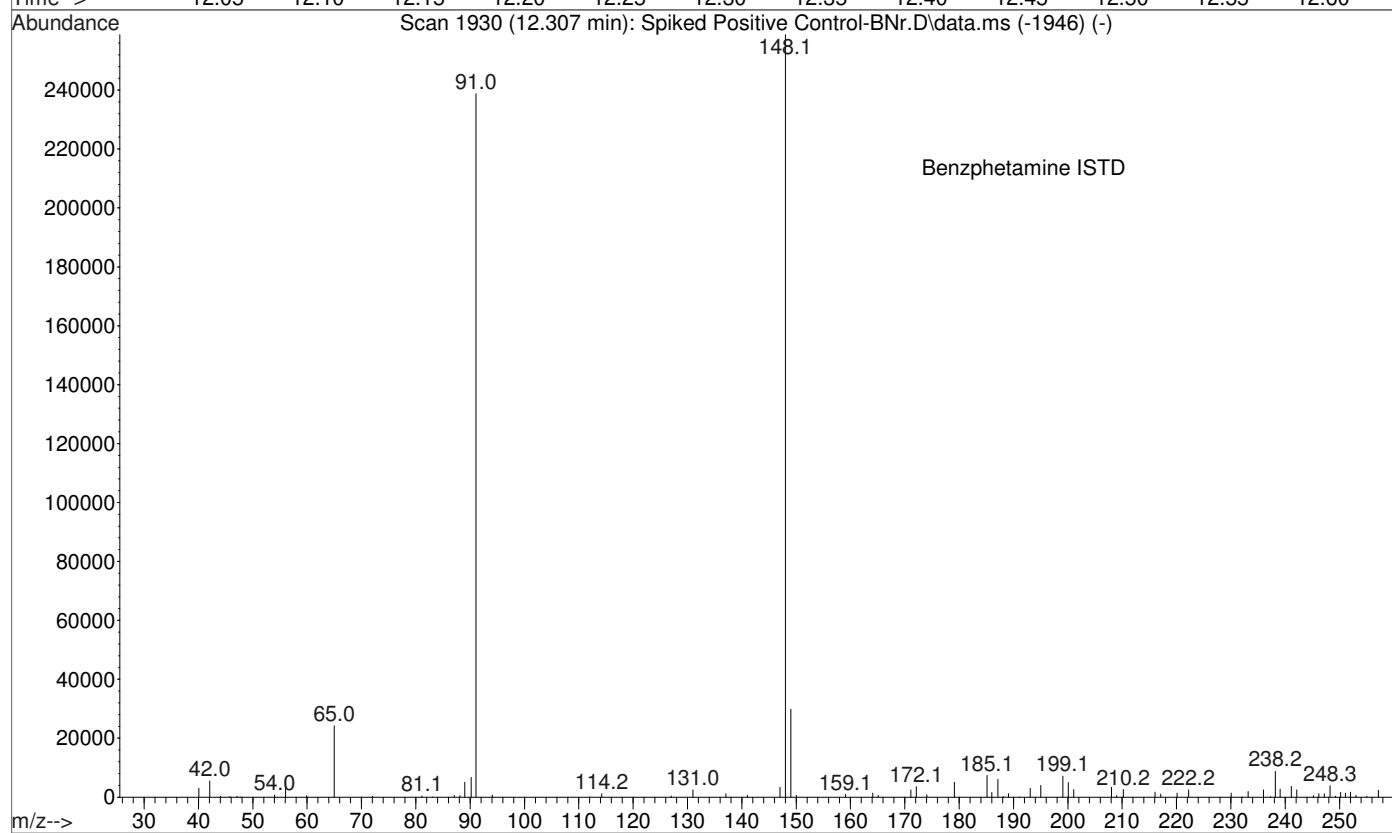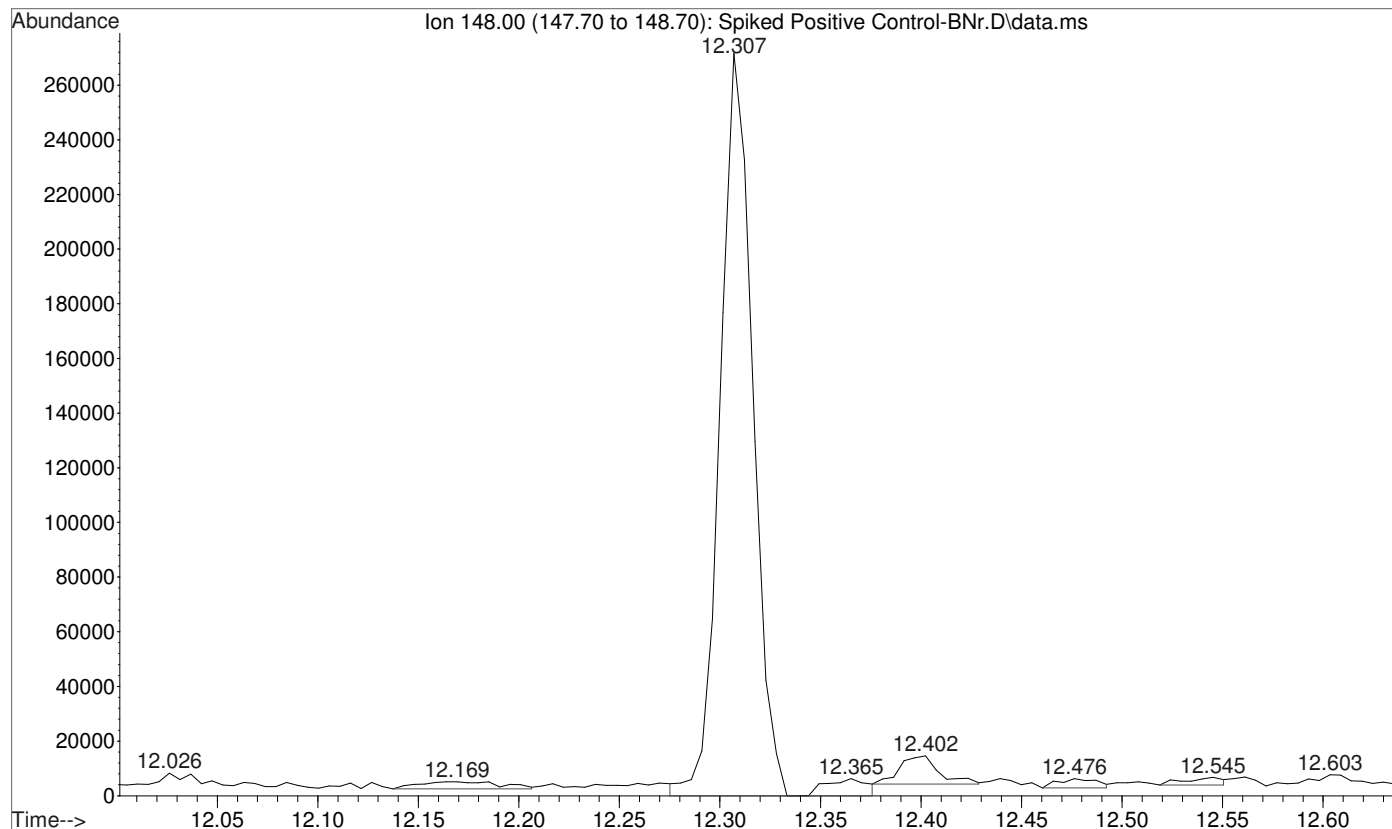



File :C:\gcms\1\data\Blood\100215\Reinjection Longer GC Method\Spi
... ked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 03 Oct 2015 02:34 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

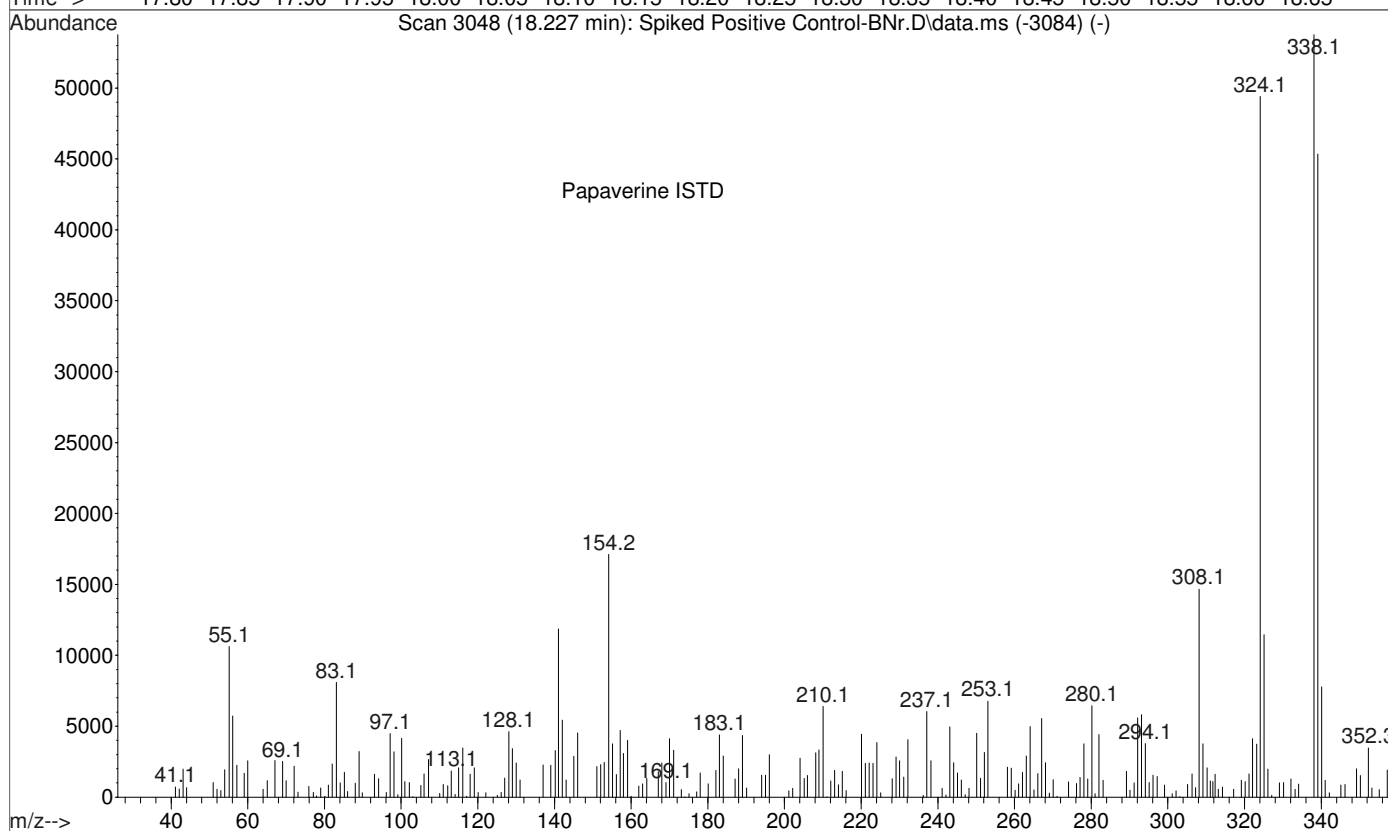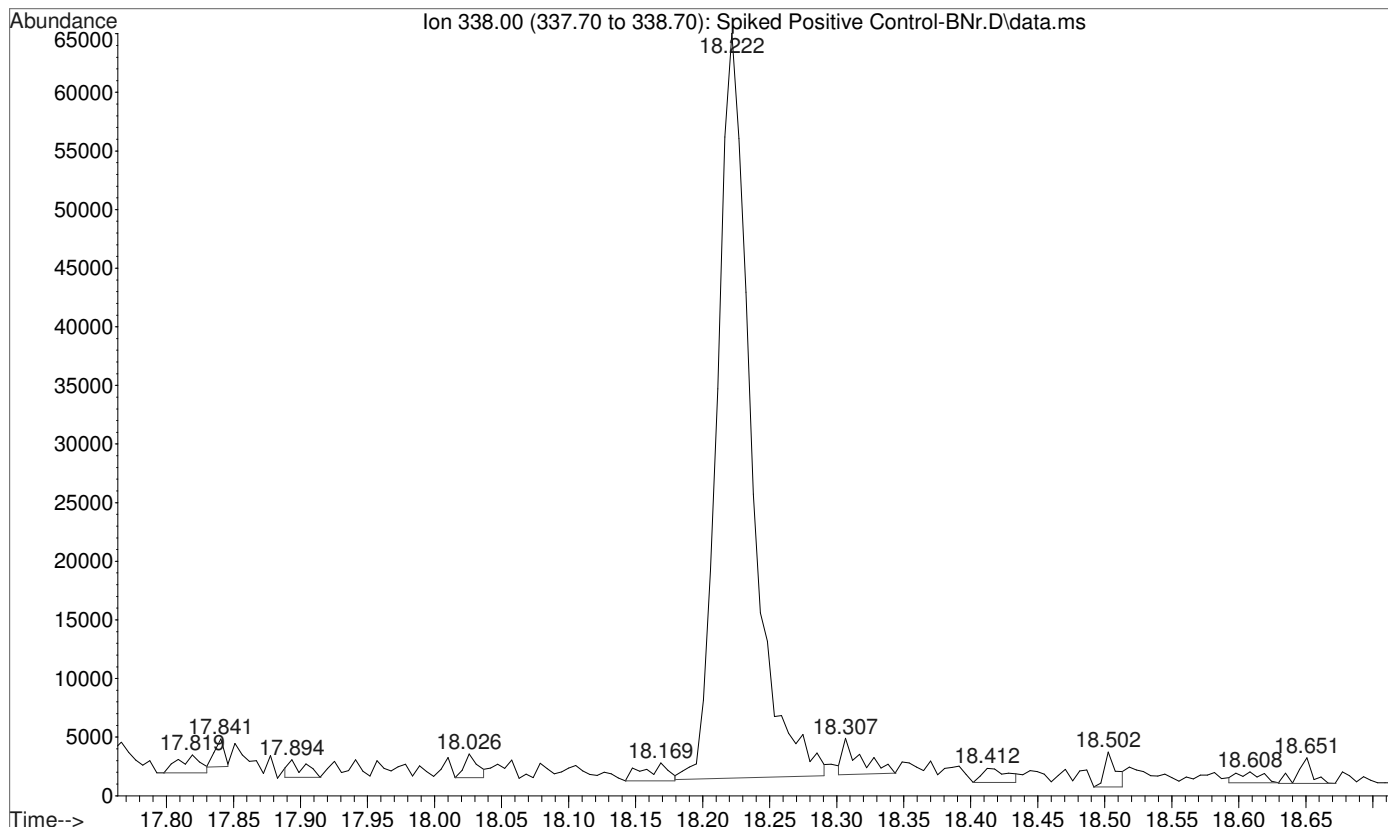



File :C:\gcms\1\data\Blood\100215\Reinjection Longer GC Method\Spi
... ked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 03 Oct 2015 02:34 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

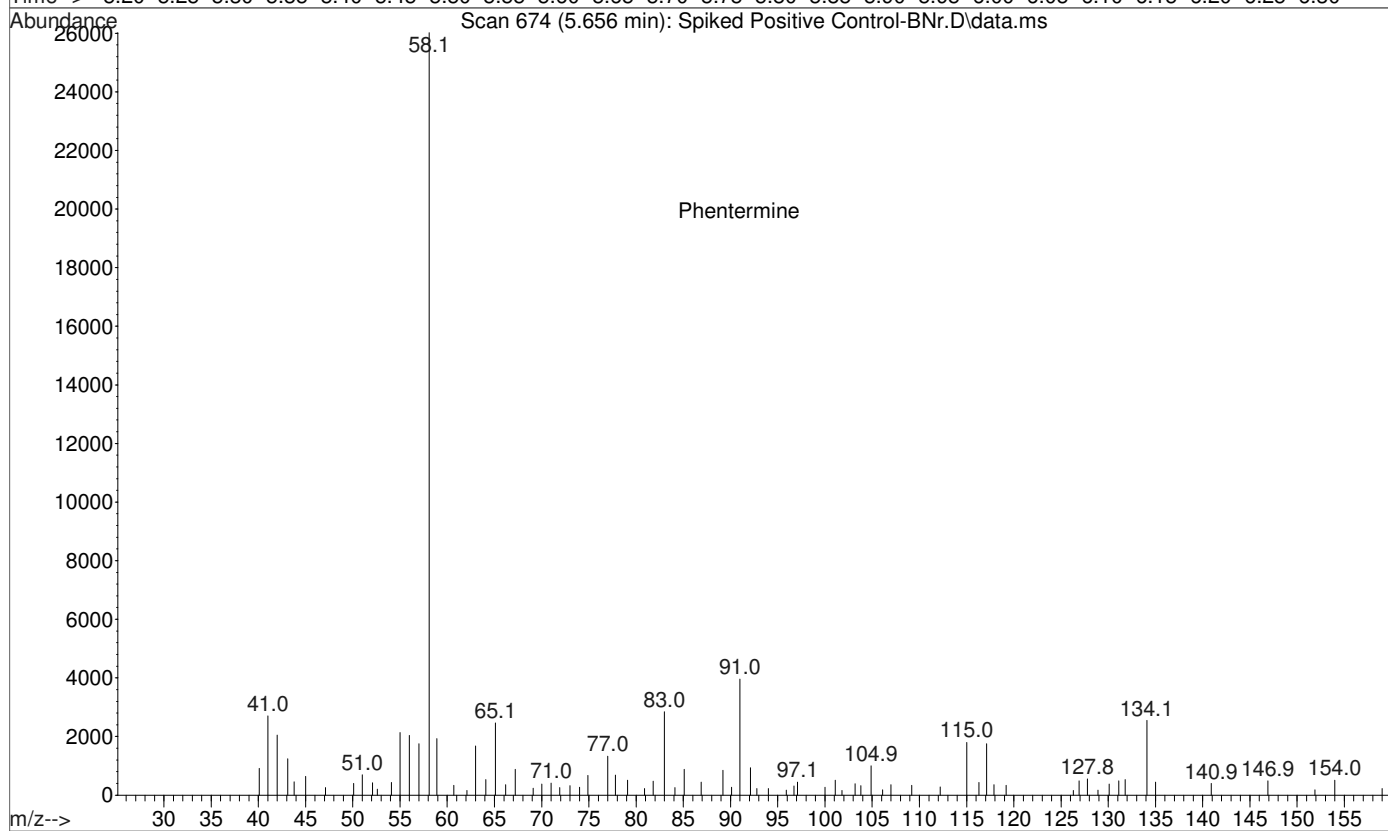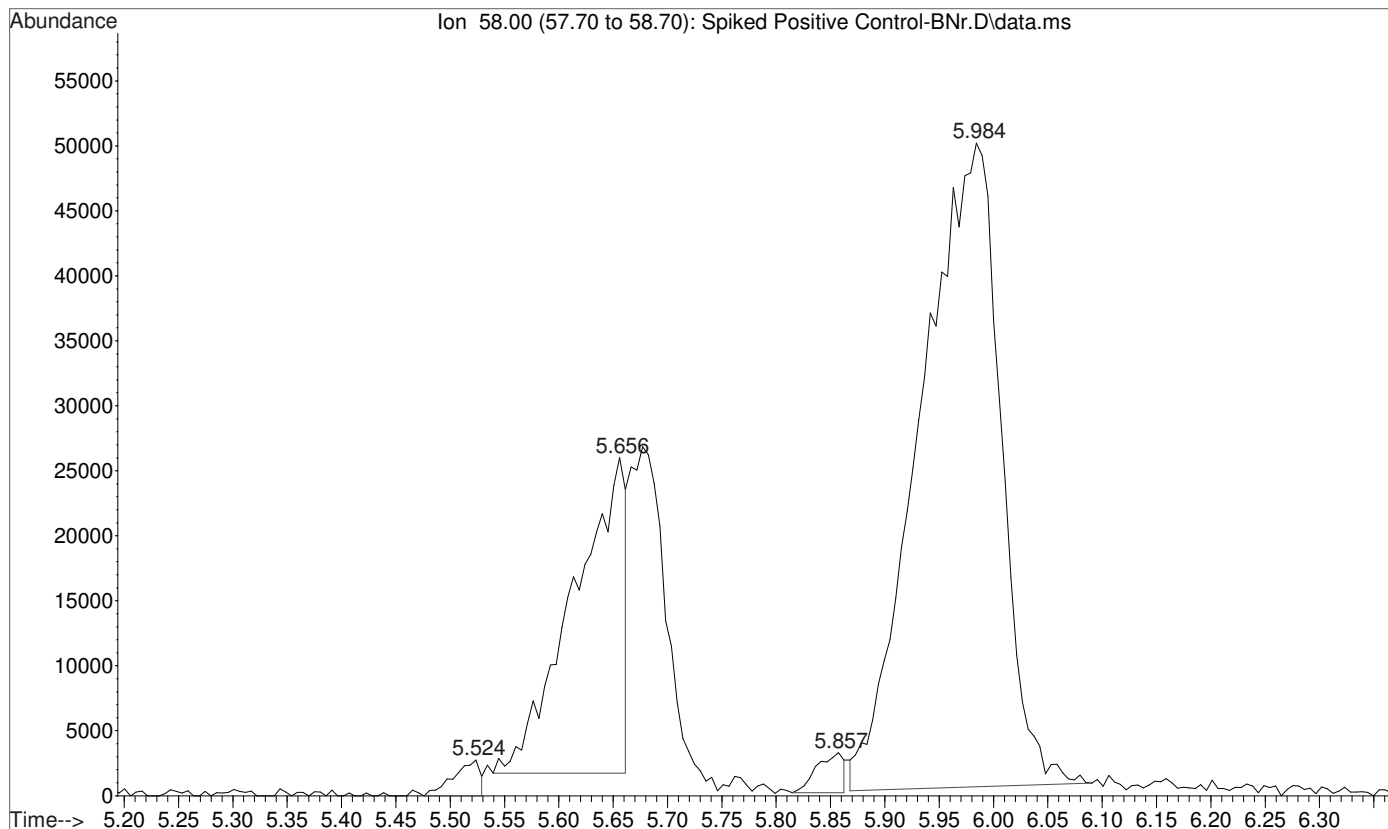



File :C:\gcms\1\data\Blood\100215\Reinjection Longer GC Method\Spi
... ked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 03 Oct 2015 02:34 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

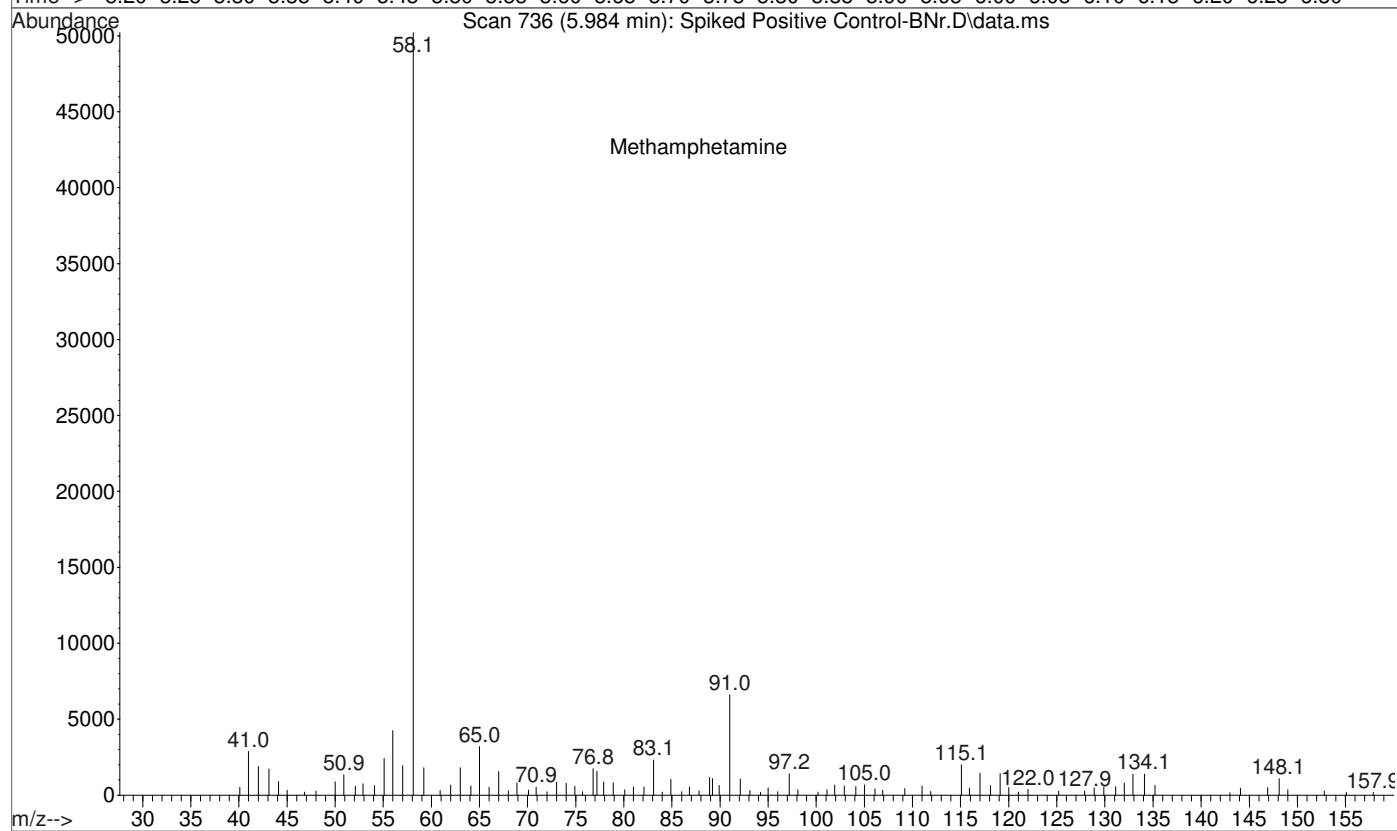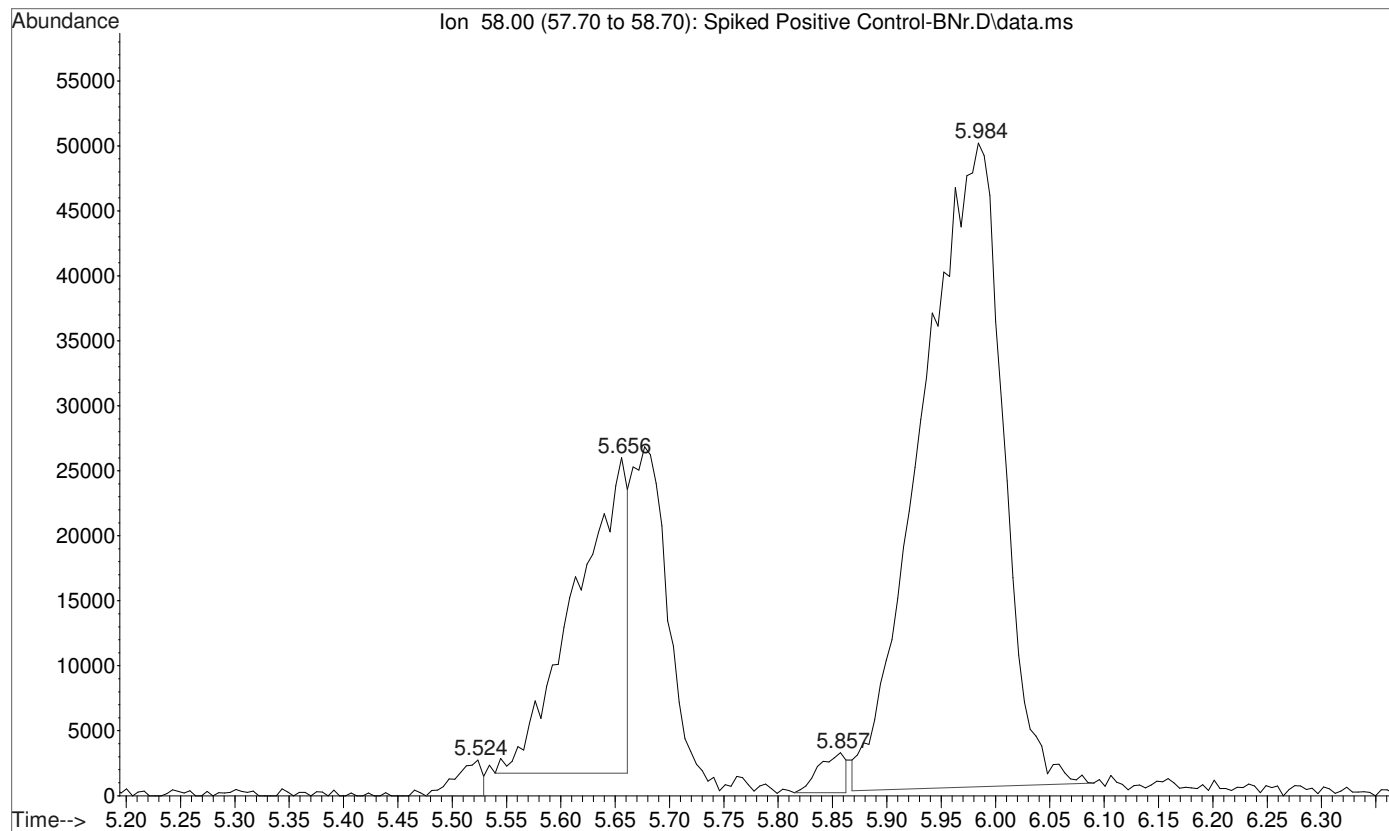



File :C:\gcms\1\data\Blood\100215\Reinjection Longer GC Method\Spi
... ked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 03 Oct 2015 02:34 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

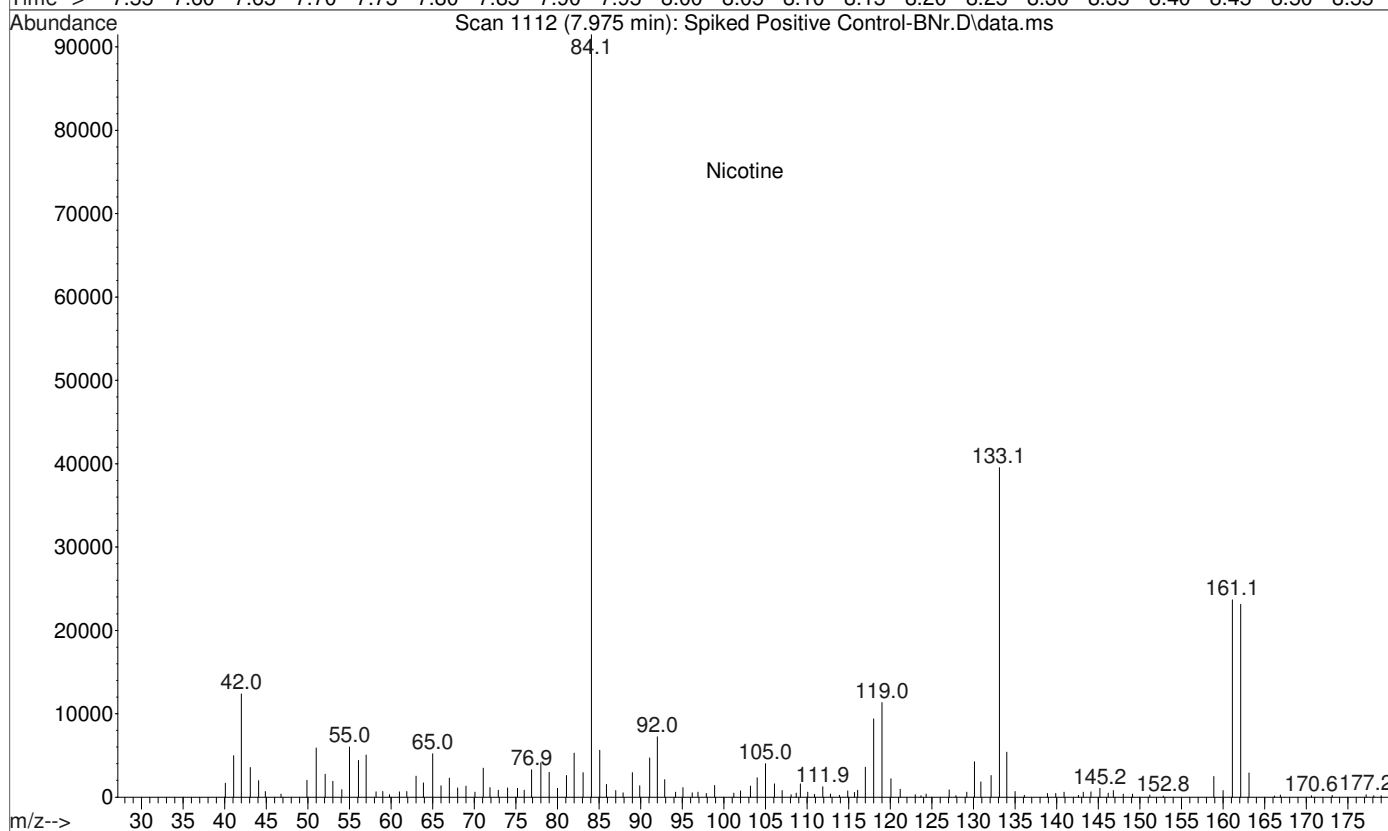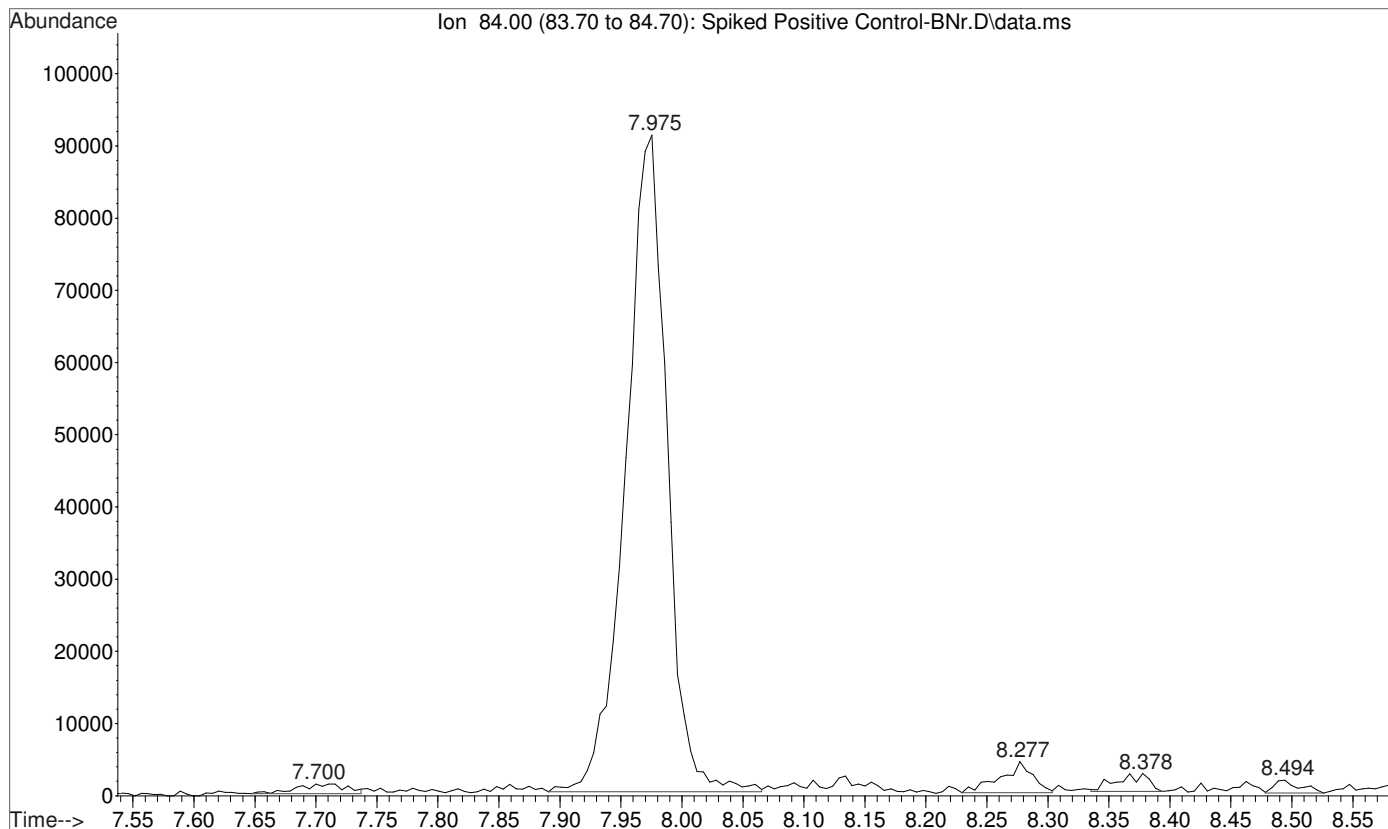



File :C:\gcms\1\data\Blood\100215\Reinjection Longer GC Method\Spi
... ked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 03 Oct 2015 02:34 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

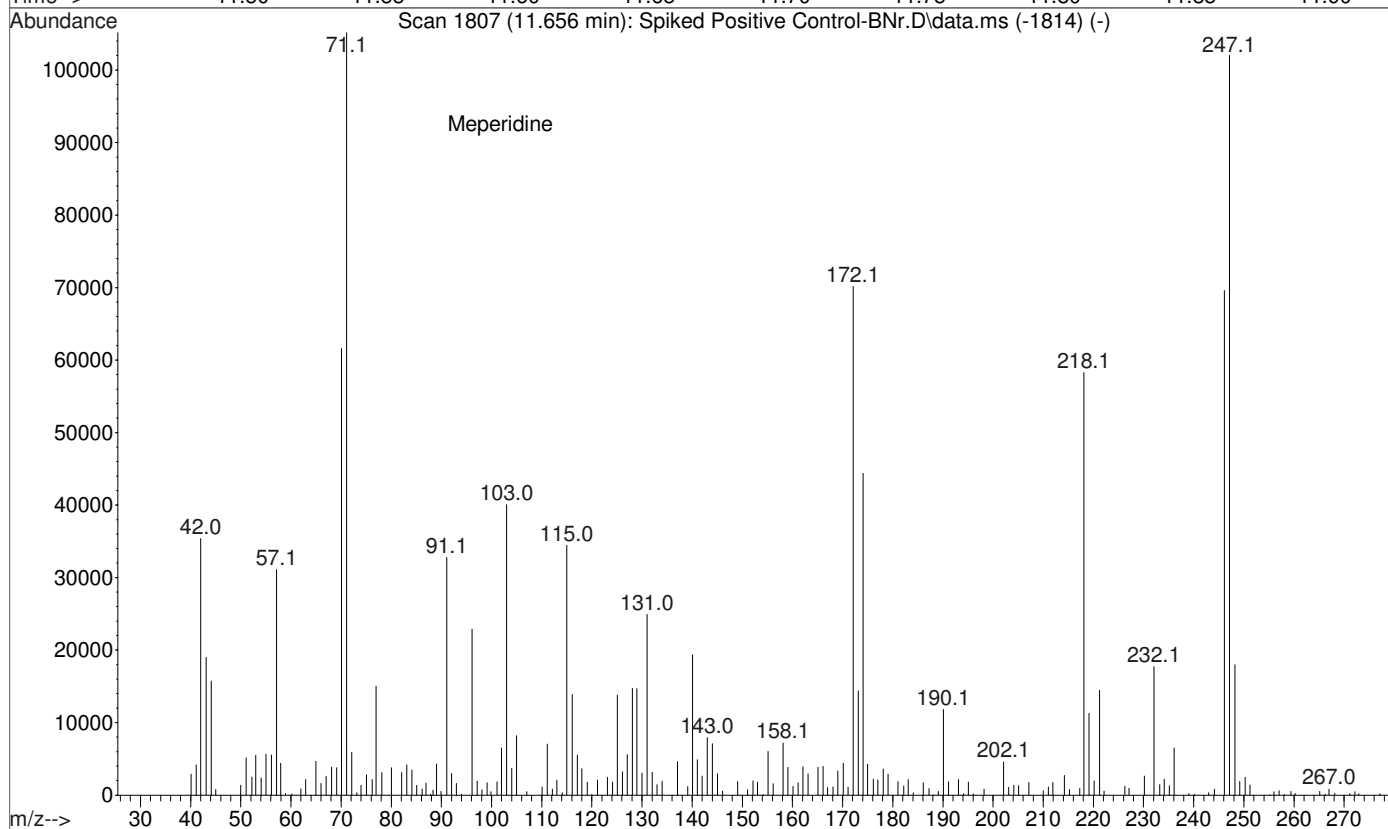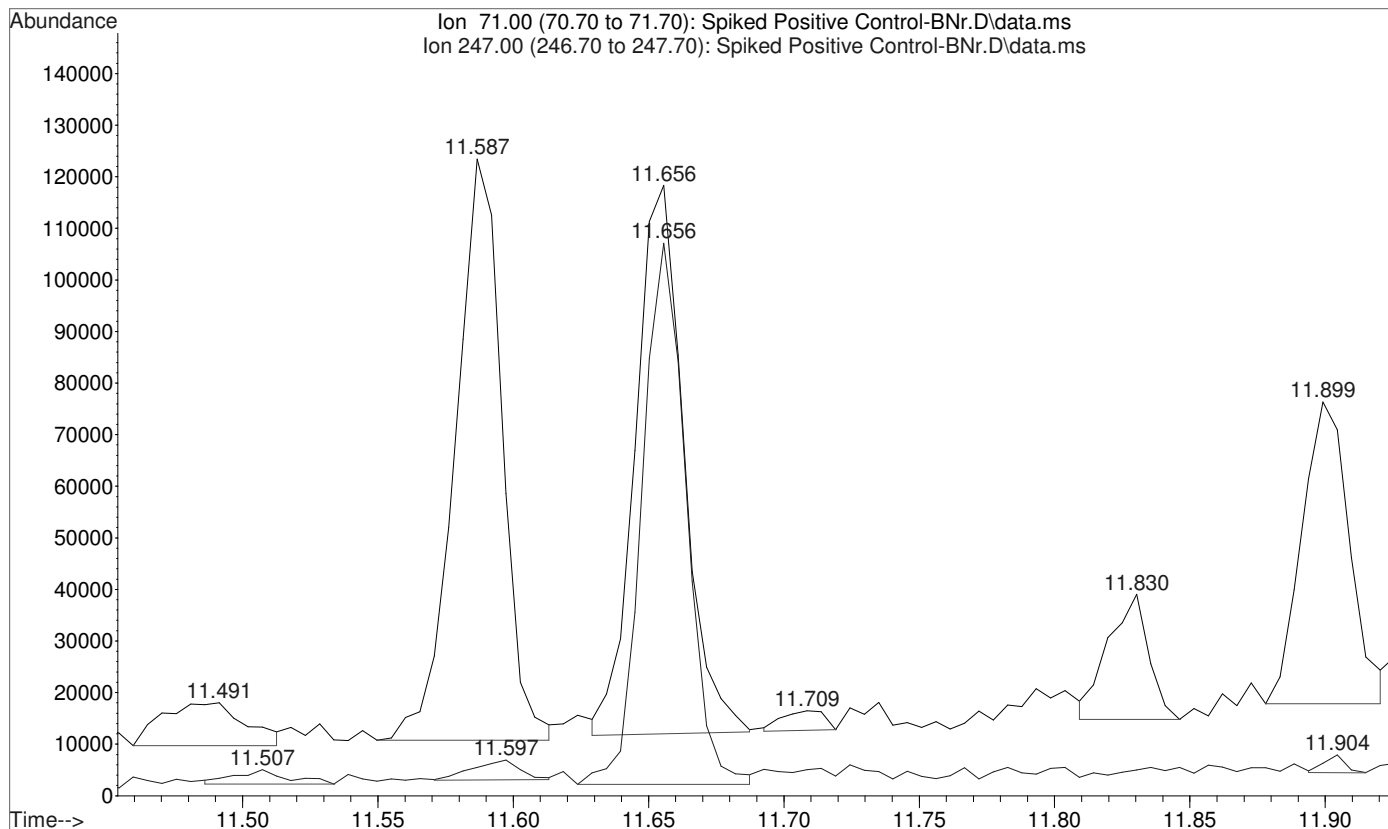



File :C:\gcms\1\data\Blood\100215\Reinjection Longer GC Method\Spi
... ked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 03 Oct 2015 02:34 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

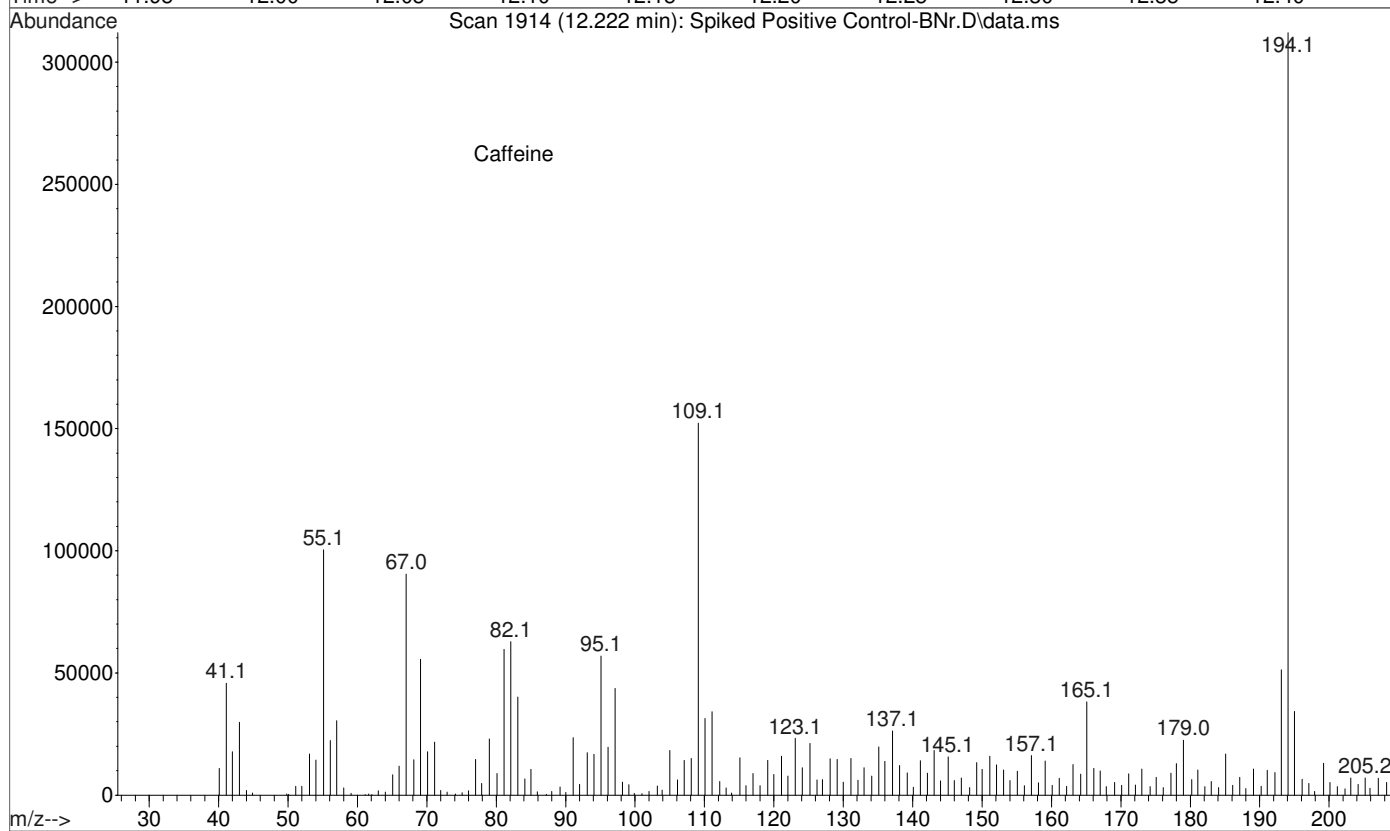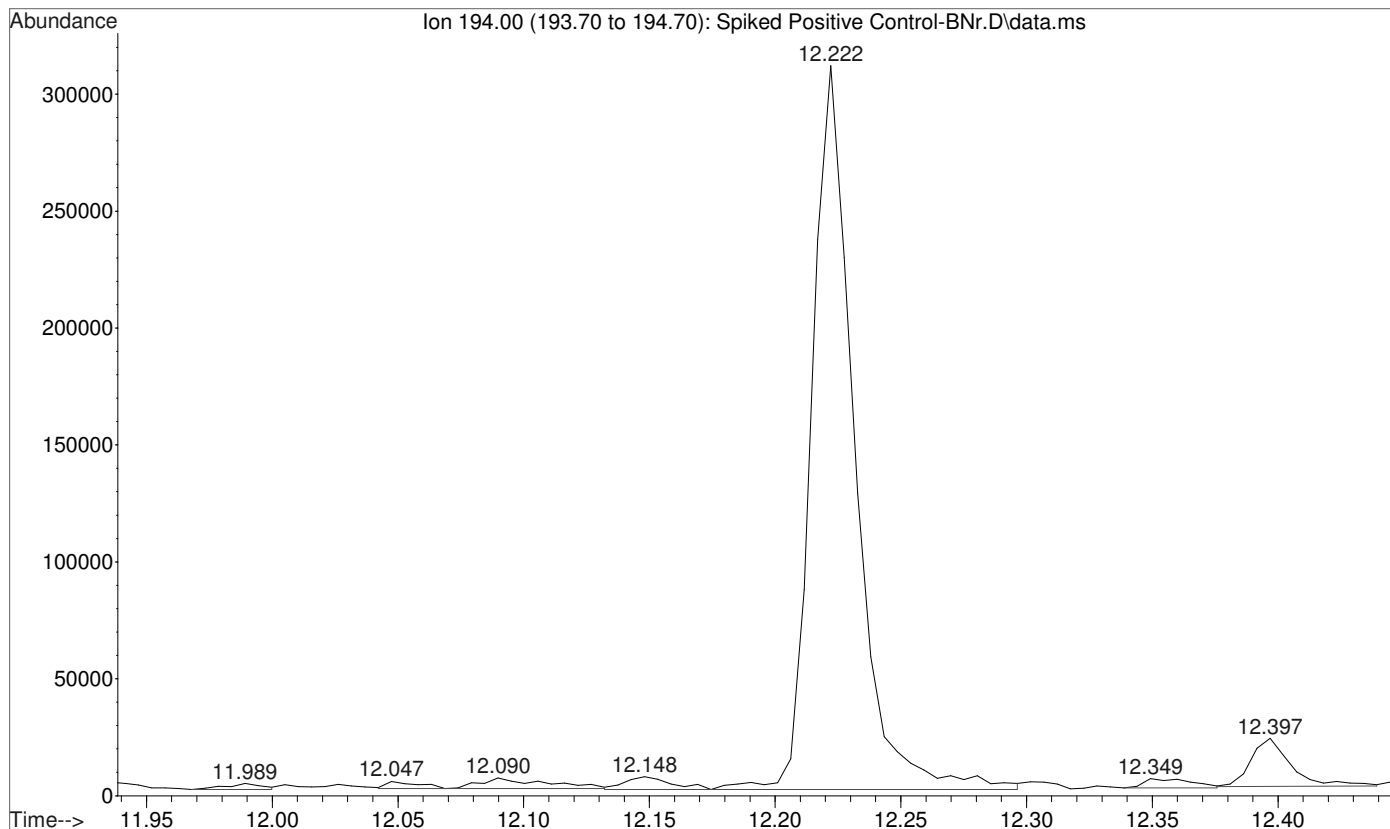



File :C:\gcms\1\data\Blood\100215\Reinjection Longer GC Method\Spi
... ked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 03 Oct 2015 02:34 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

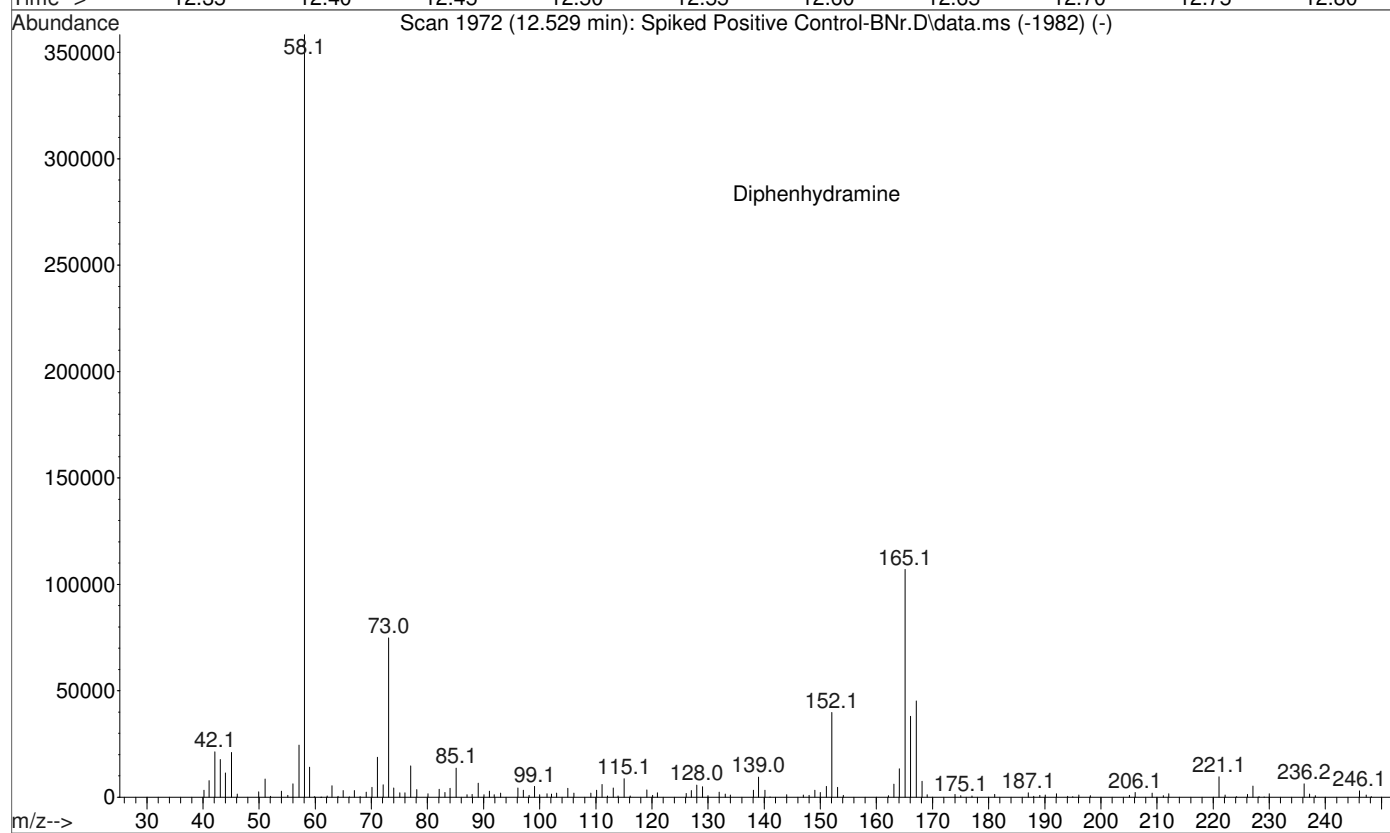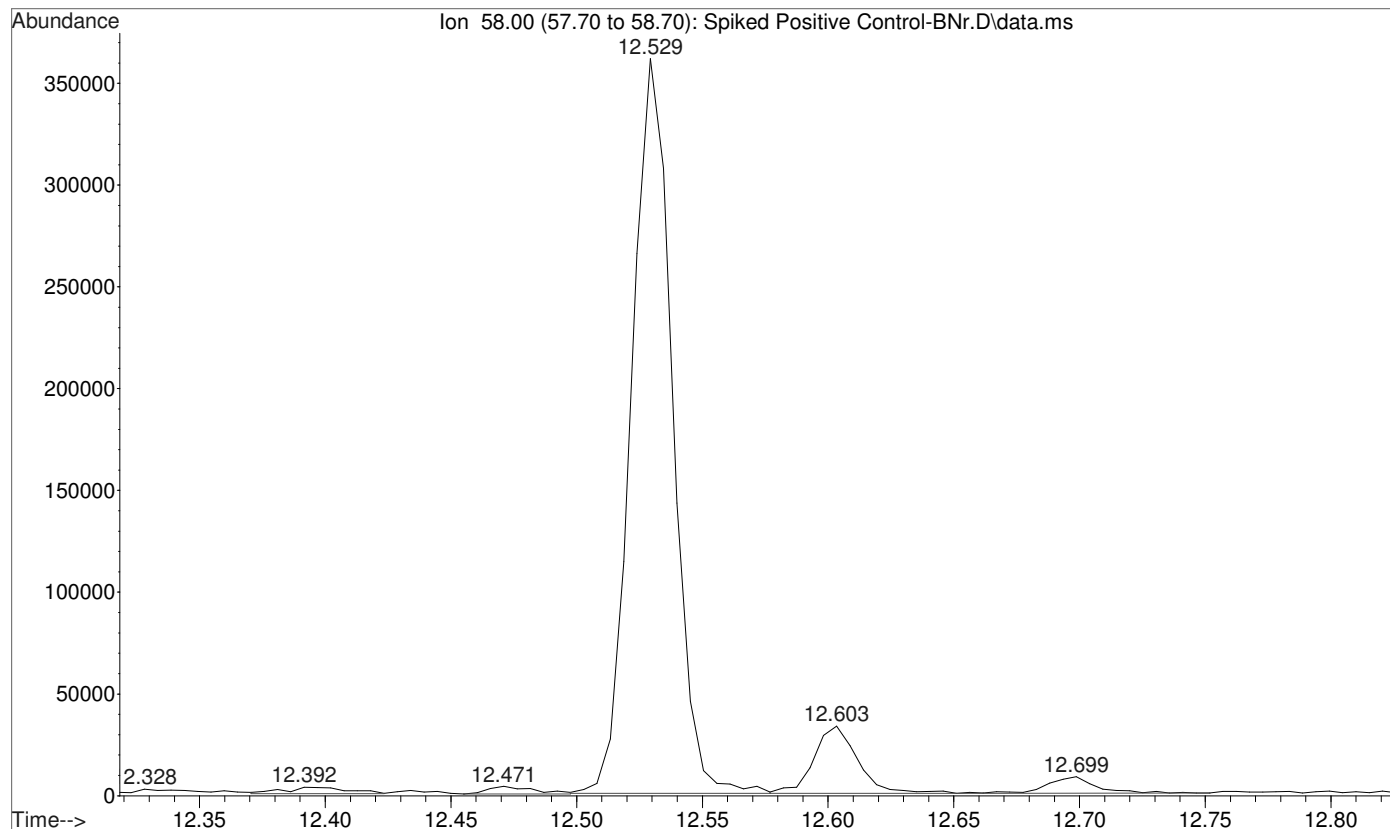



File :C:\gcms\1\data\Blood\100215\Reinjection Longer GC Method\Spi
... ked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 03 Oct 2015 02:34 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

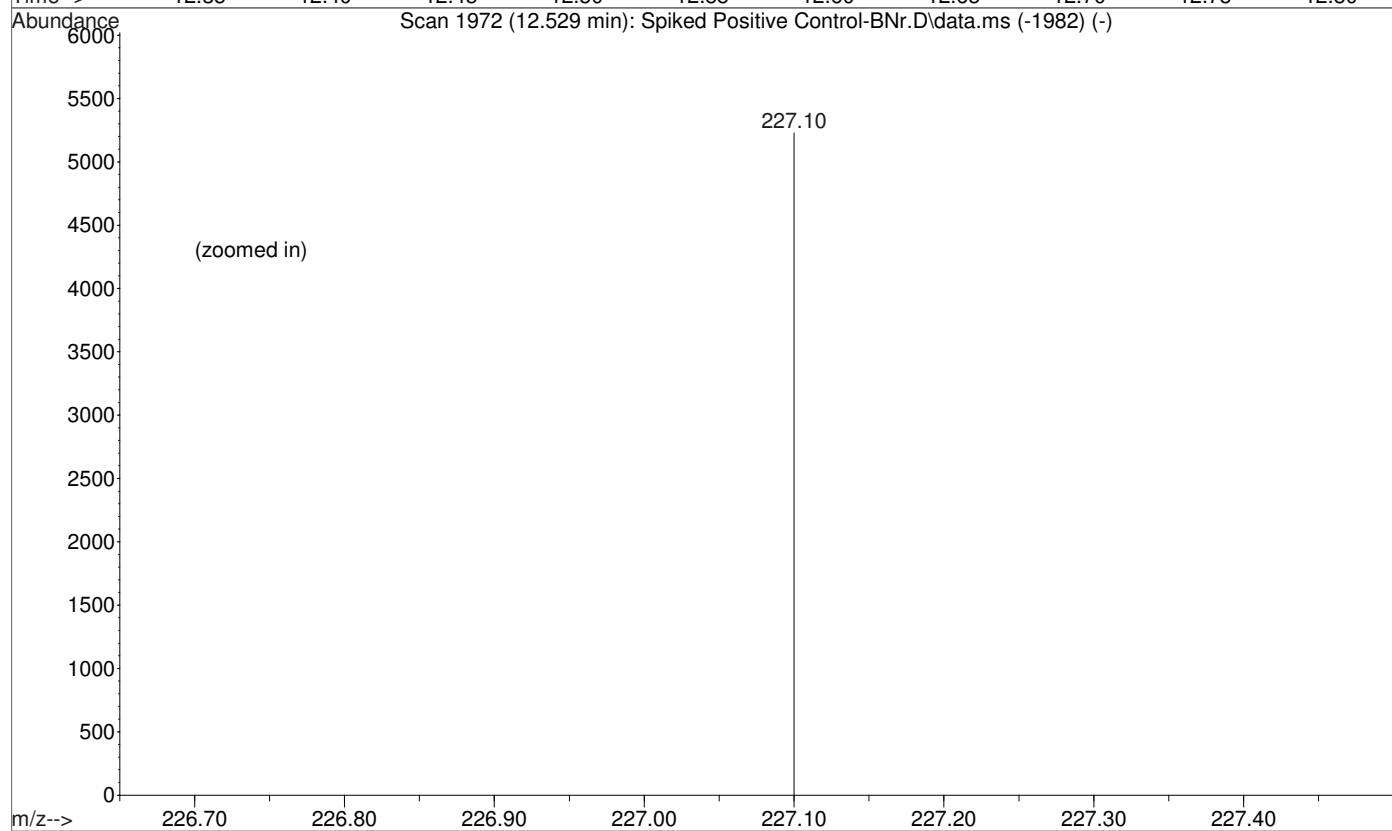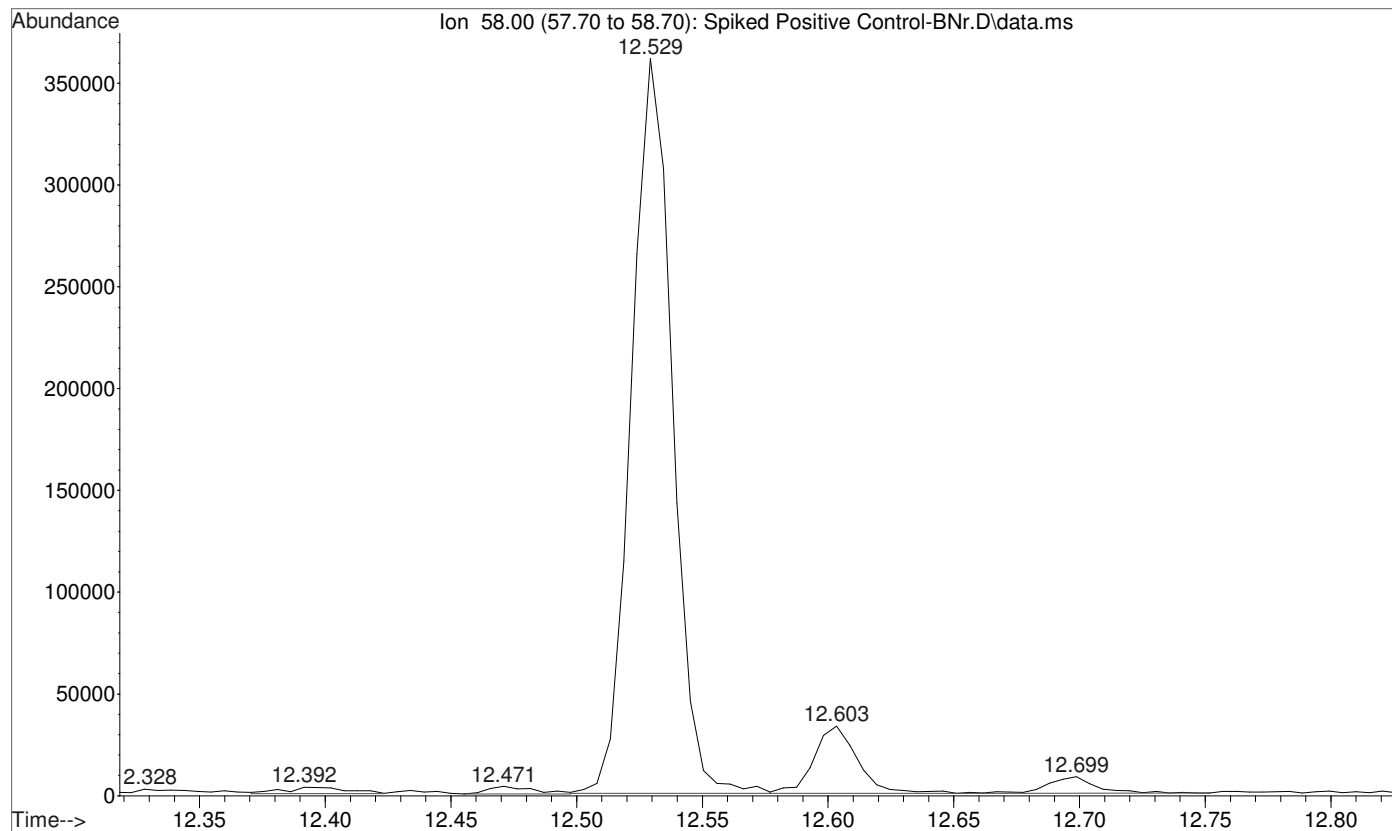



File :C:\gcms\1\data\Blood\100215\Reinjection Longer GC Method\Spi
... ked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 03 Oct 2015 02:34 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

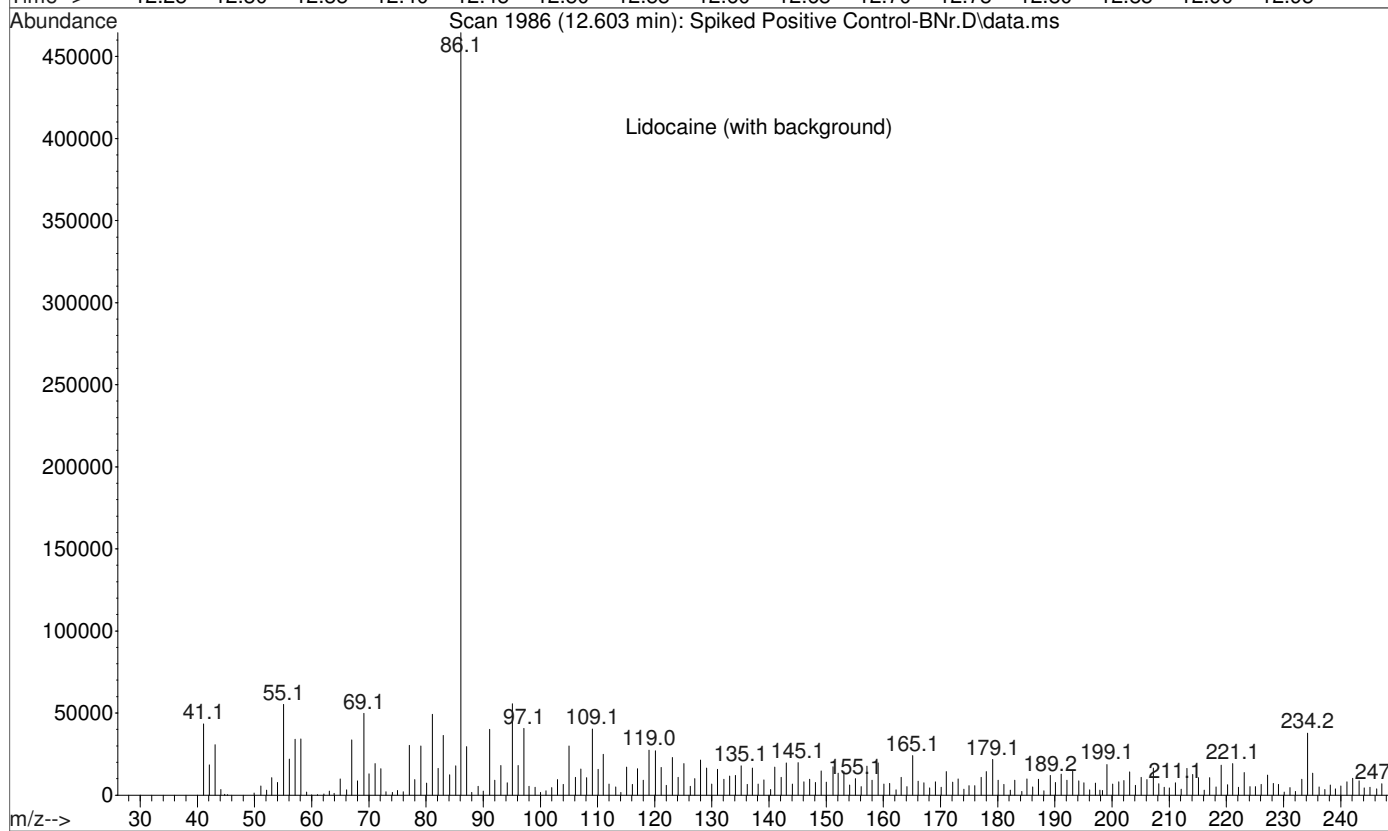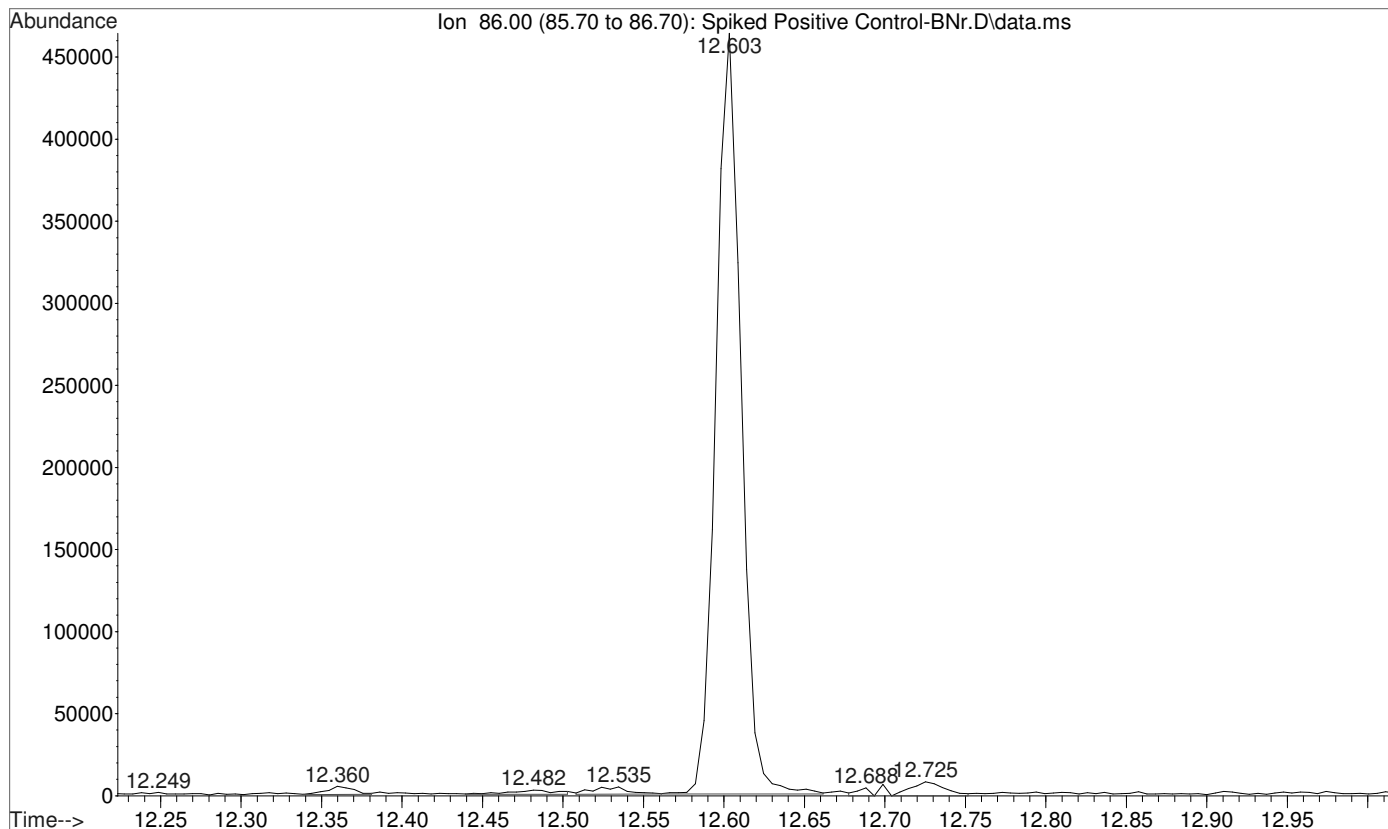



File :C:\gcms\1\data\Blood\100215\Reinjection Longer GC Method\Spi
... ked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 03 Oct 2015 02:34 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

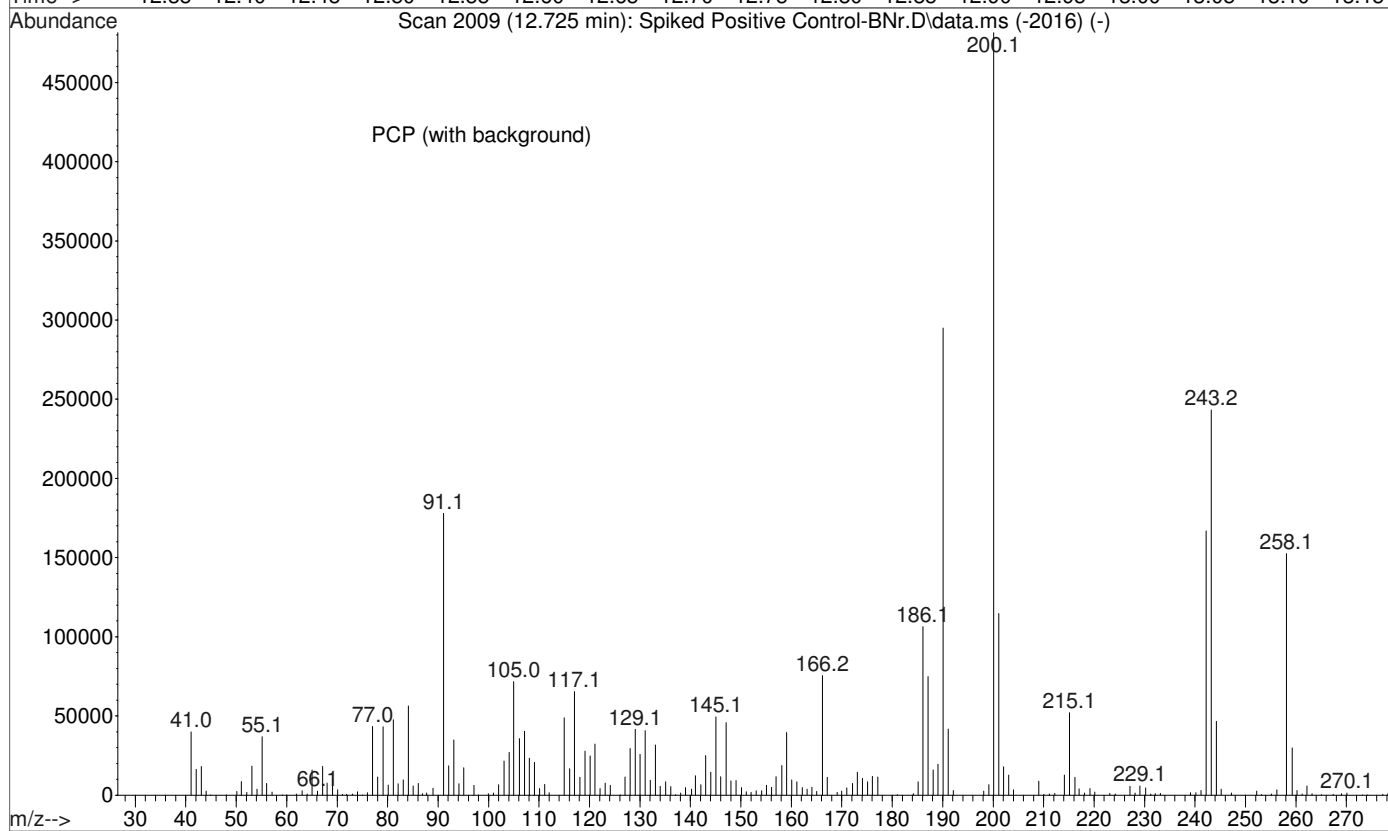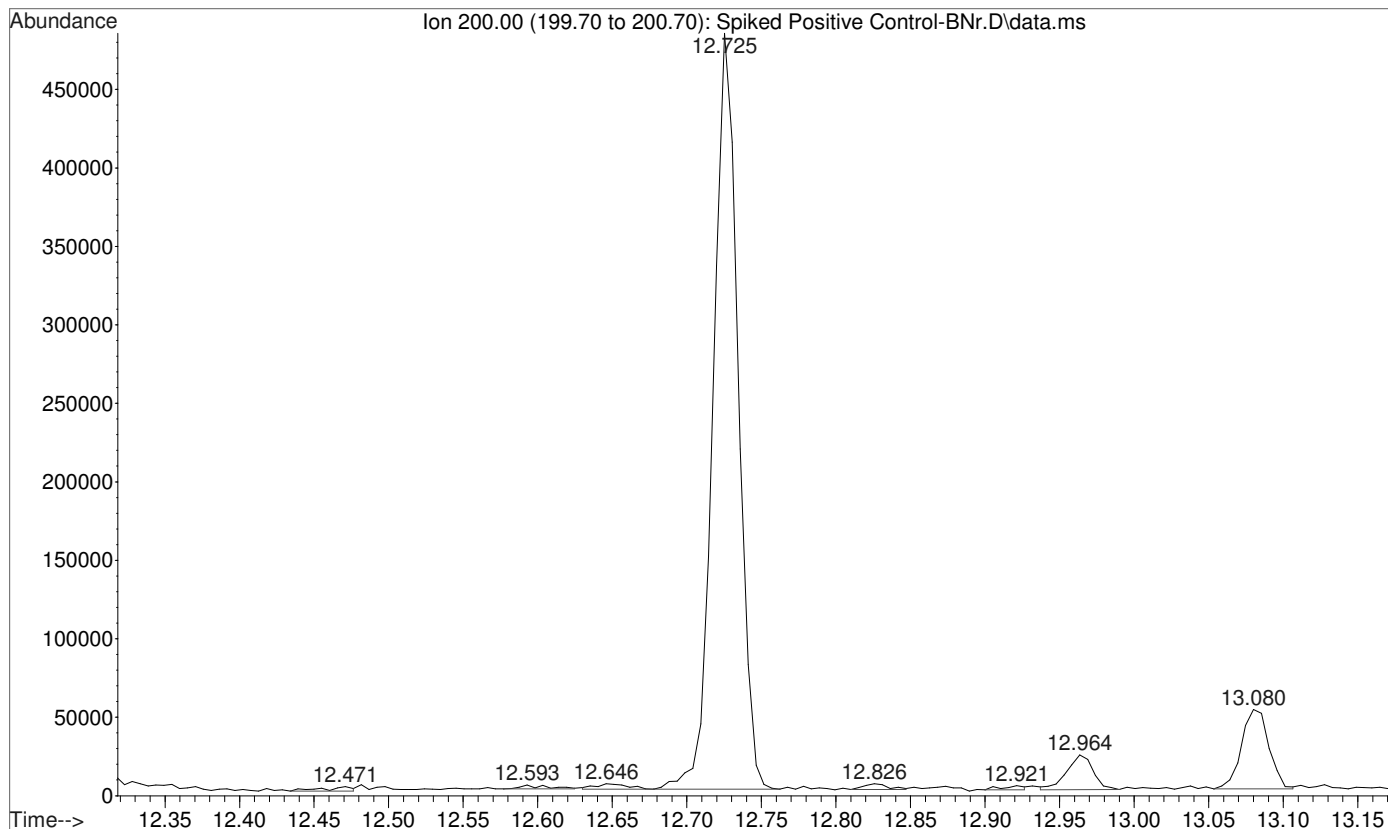



File :C:\gcms\1\data\Blood\100215\Reinjection Longer GC Method\Spi
... ked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 03 Oct 2015 02:34 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

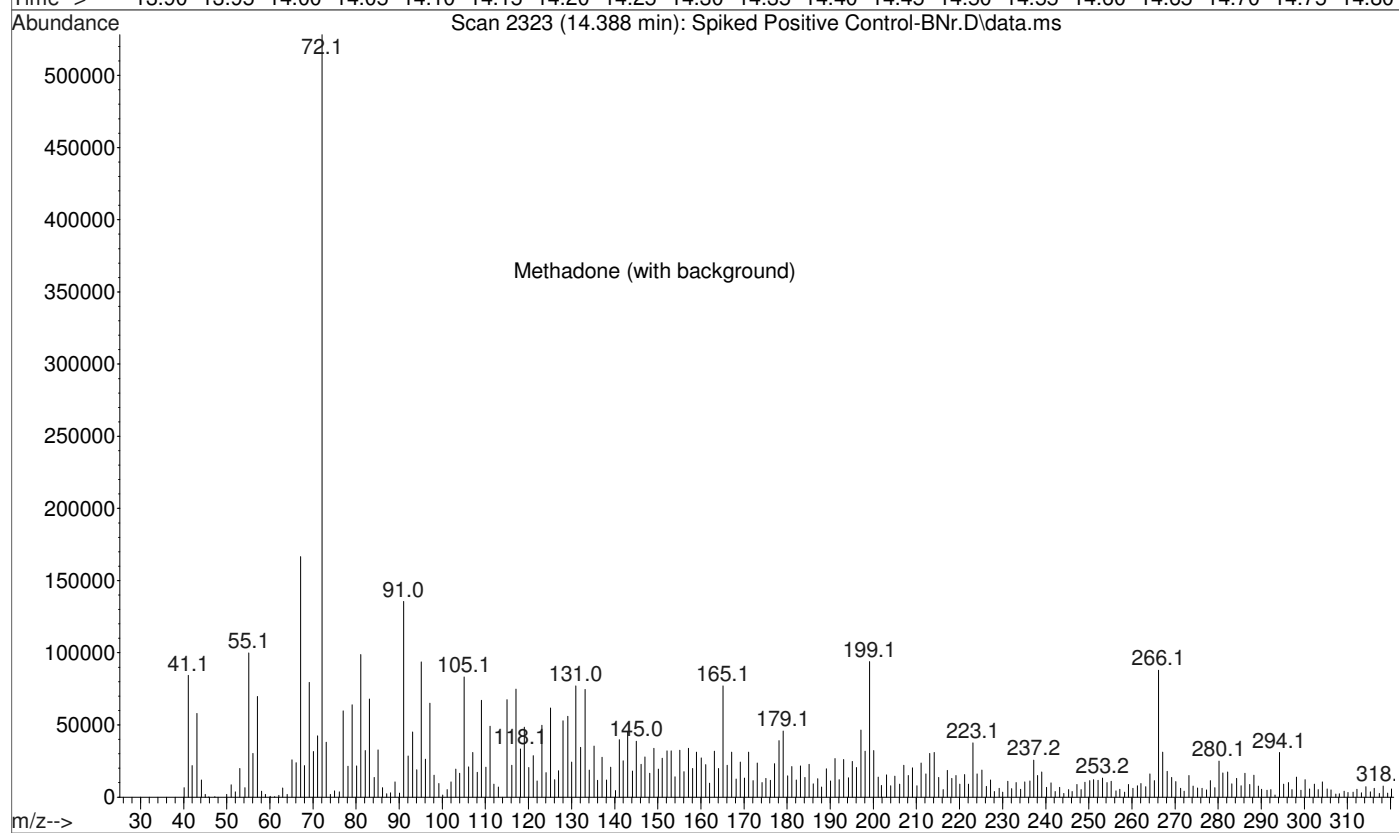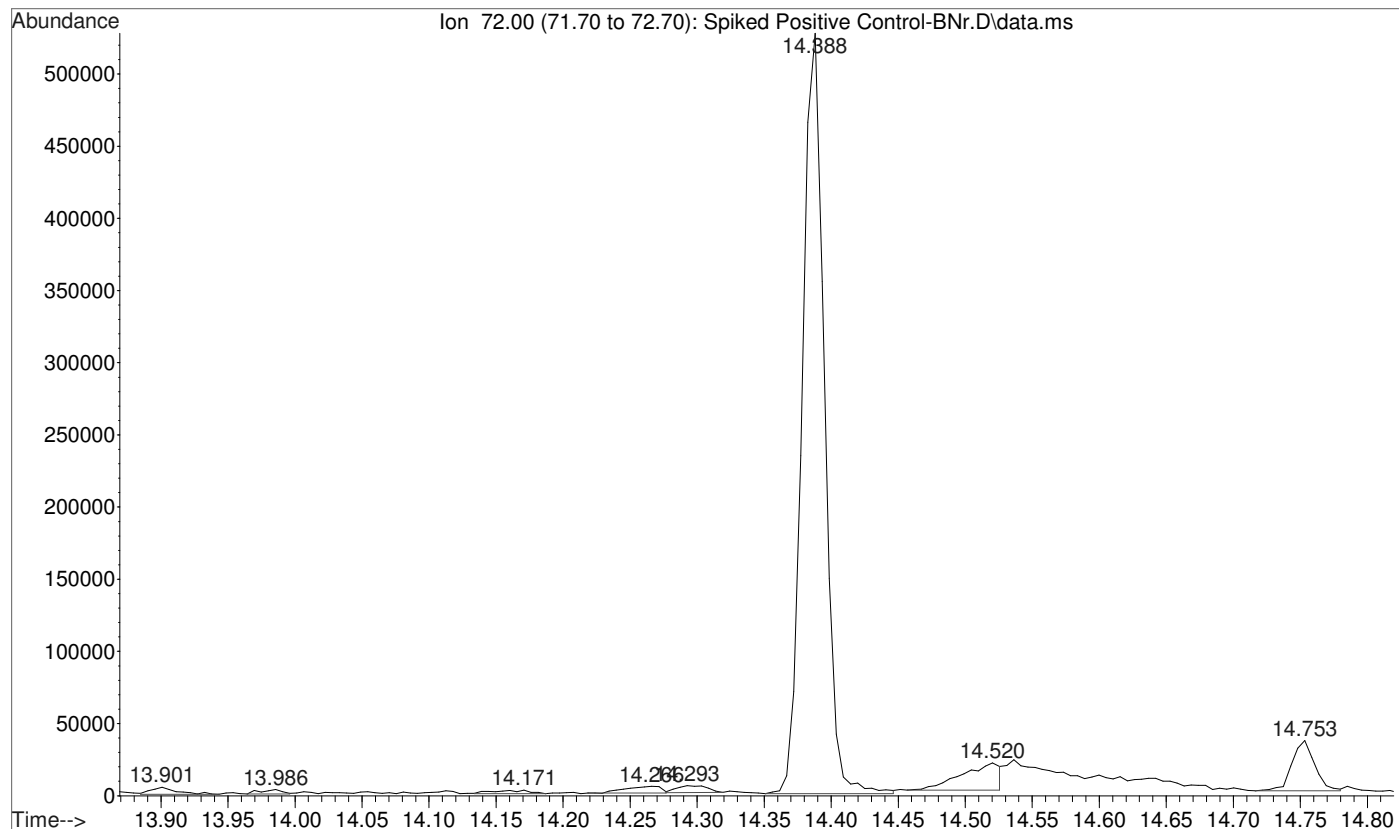



File :C:\gcms\1\data\Blood\100215\Reinjection Longer GC Method\Spi
... ked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 03 Oct 2015 02:34 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

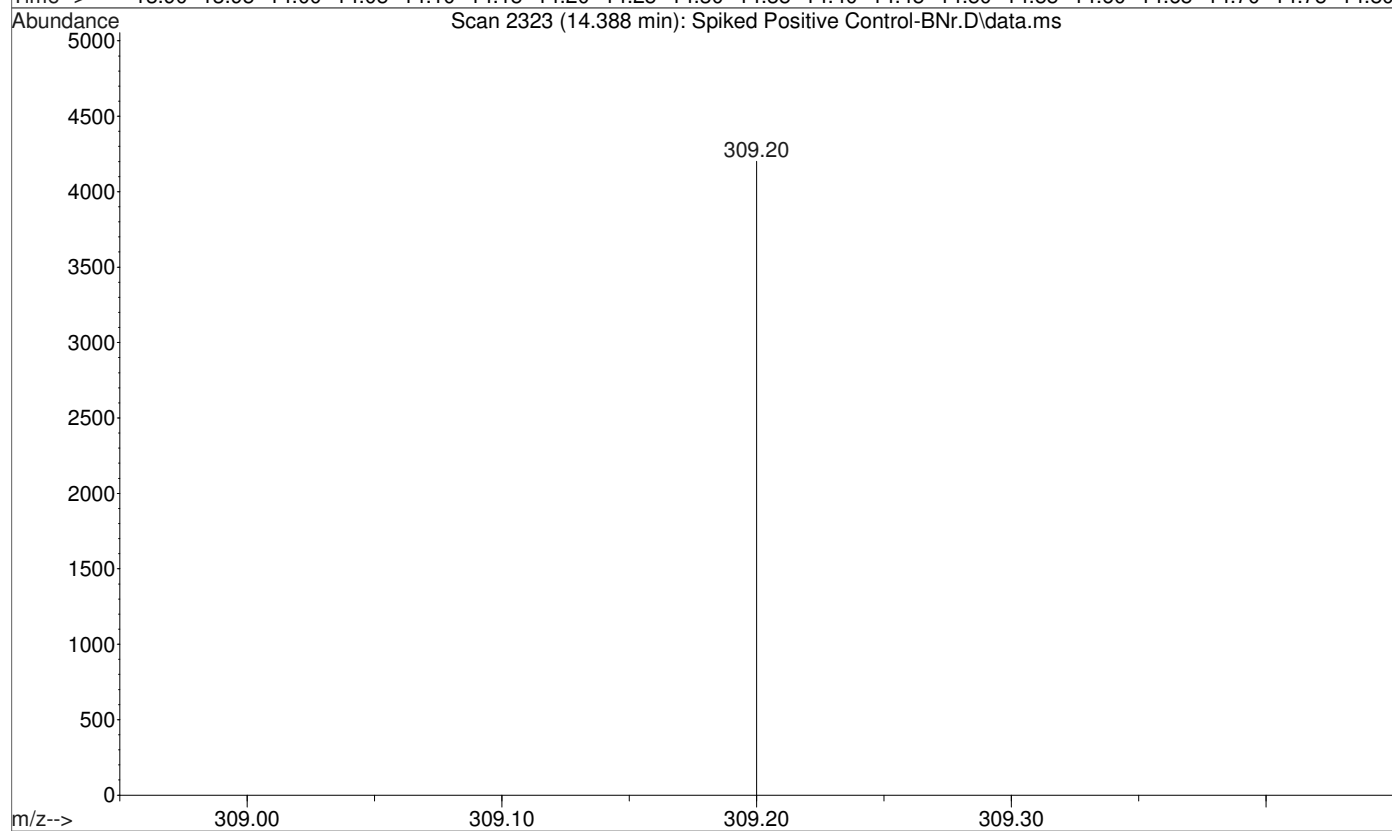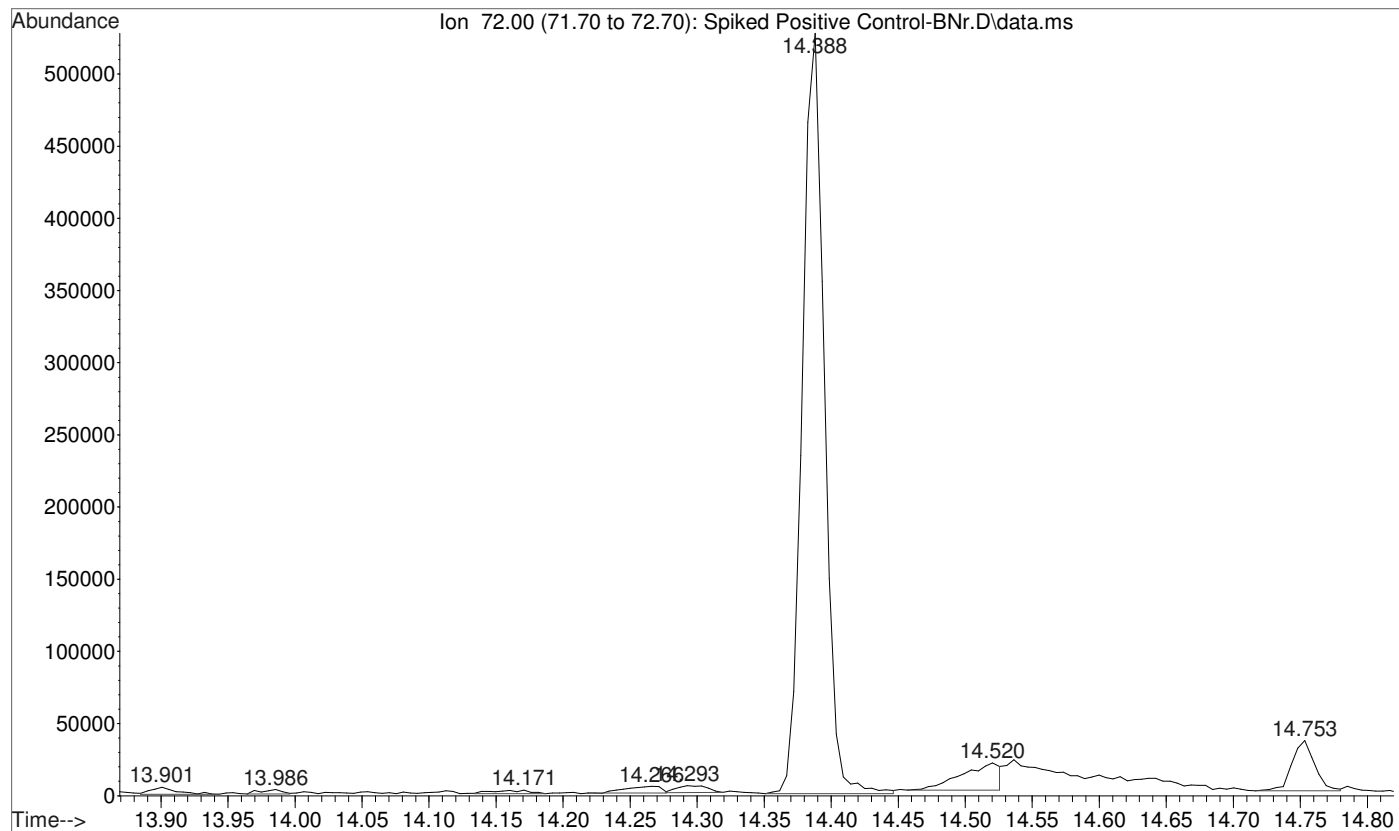



File :C:\gcms\1\data\Blood\100215\Reinjection Longer GC Method\Spi
... ked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 03 Oct 2015 02:34 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

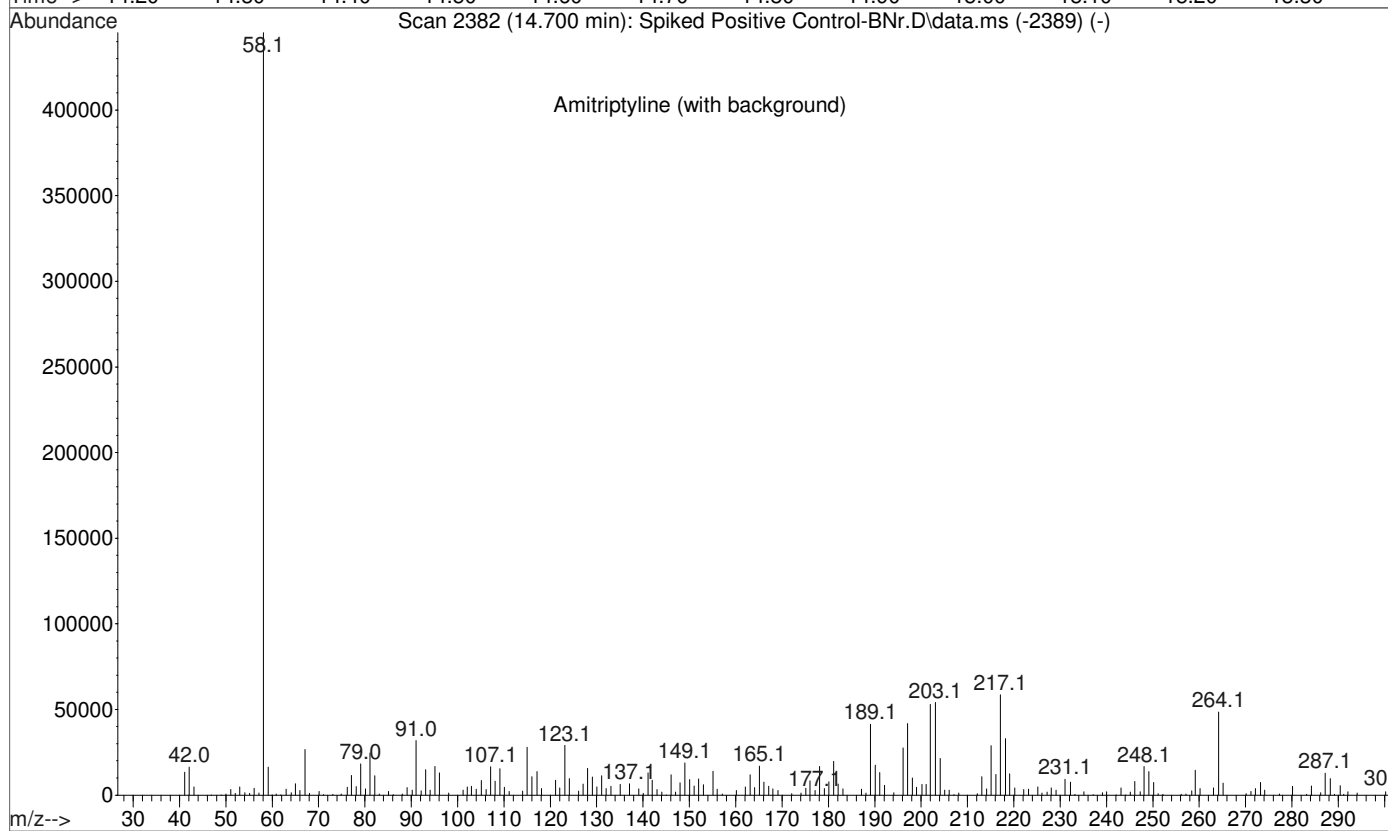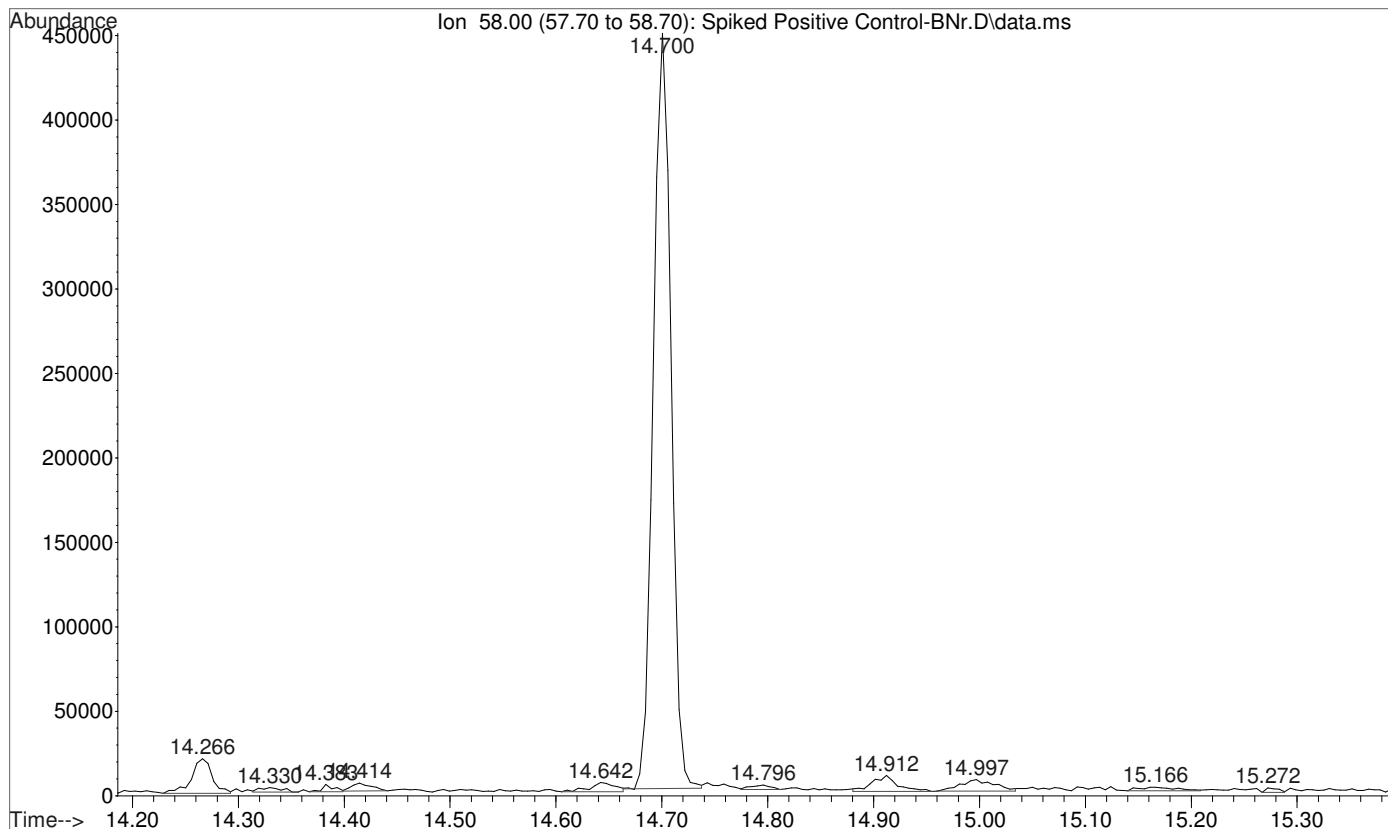




File :C:\gcms\1\data\Blood\100215\Reinjection Longer GC Method\Spi
... ked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 03 Oct 2015 02:34 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

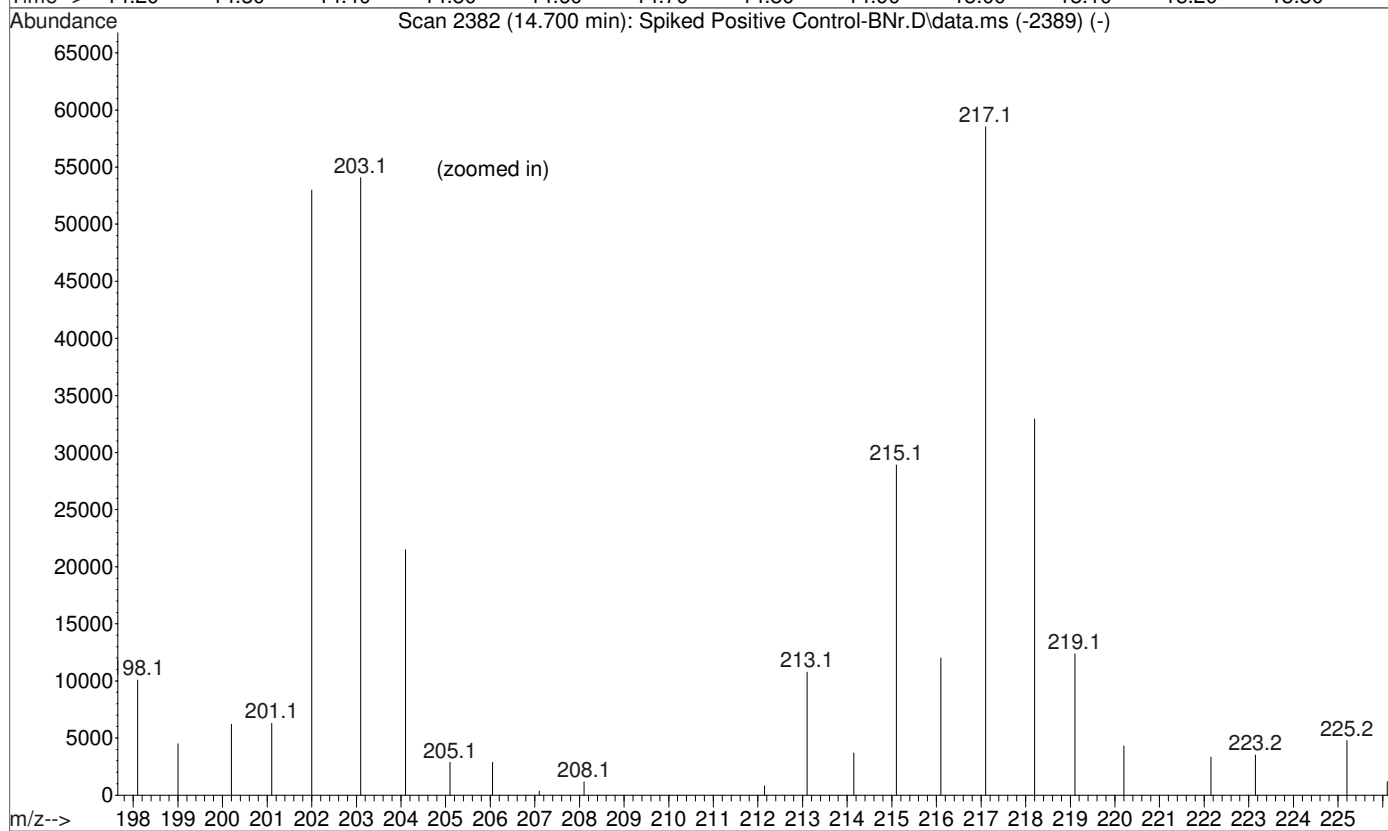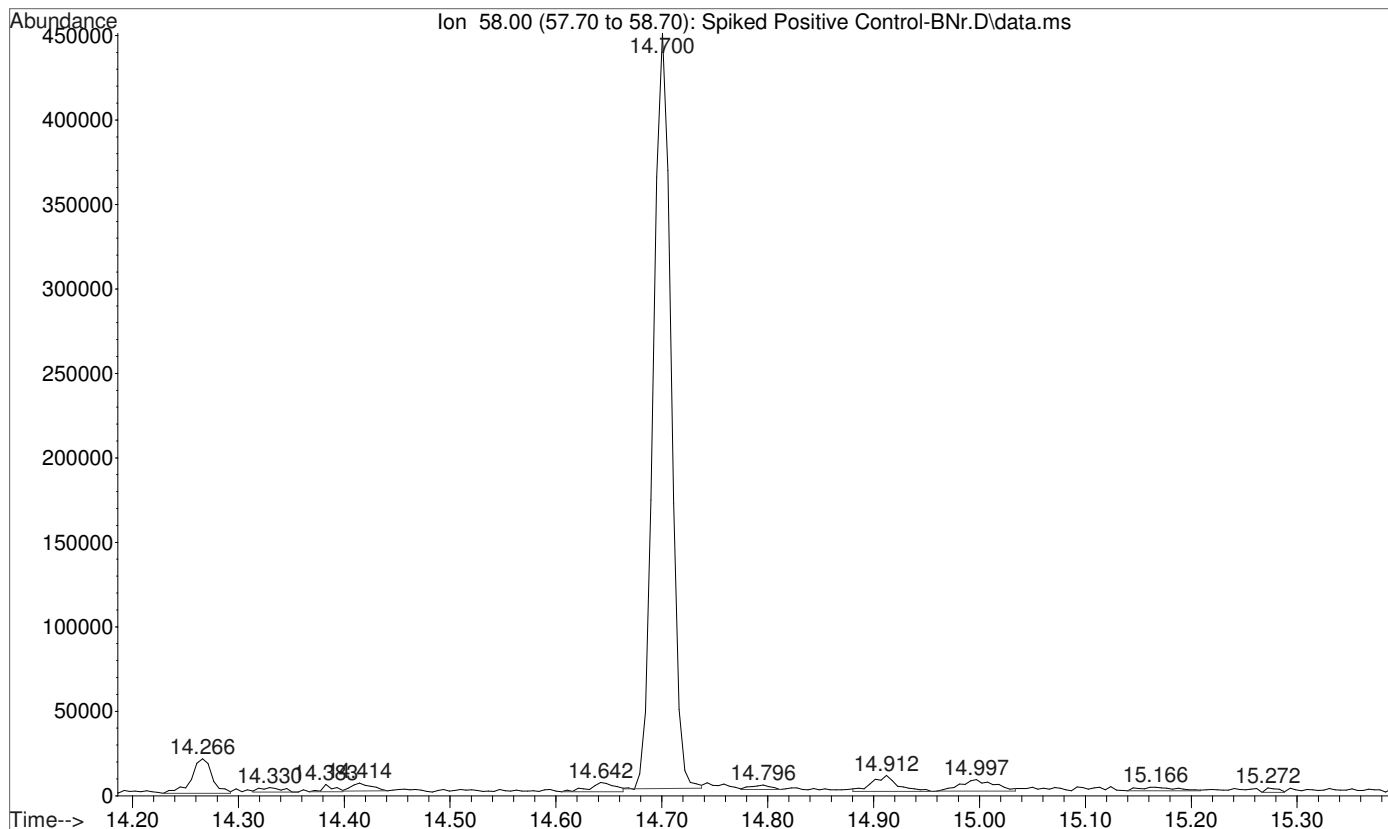



File :C:\gcms\1\data\Blood\100215\Reinjection Longer GC Method\Spi
... ked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 03 Oct 2015 02:34 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

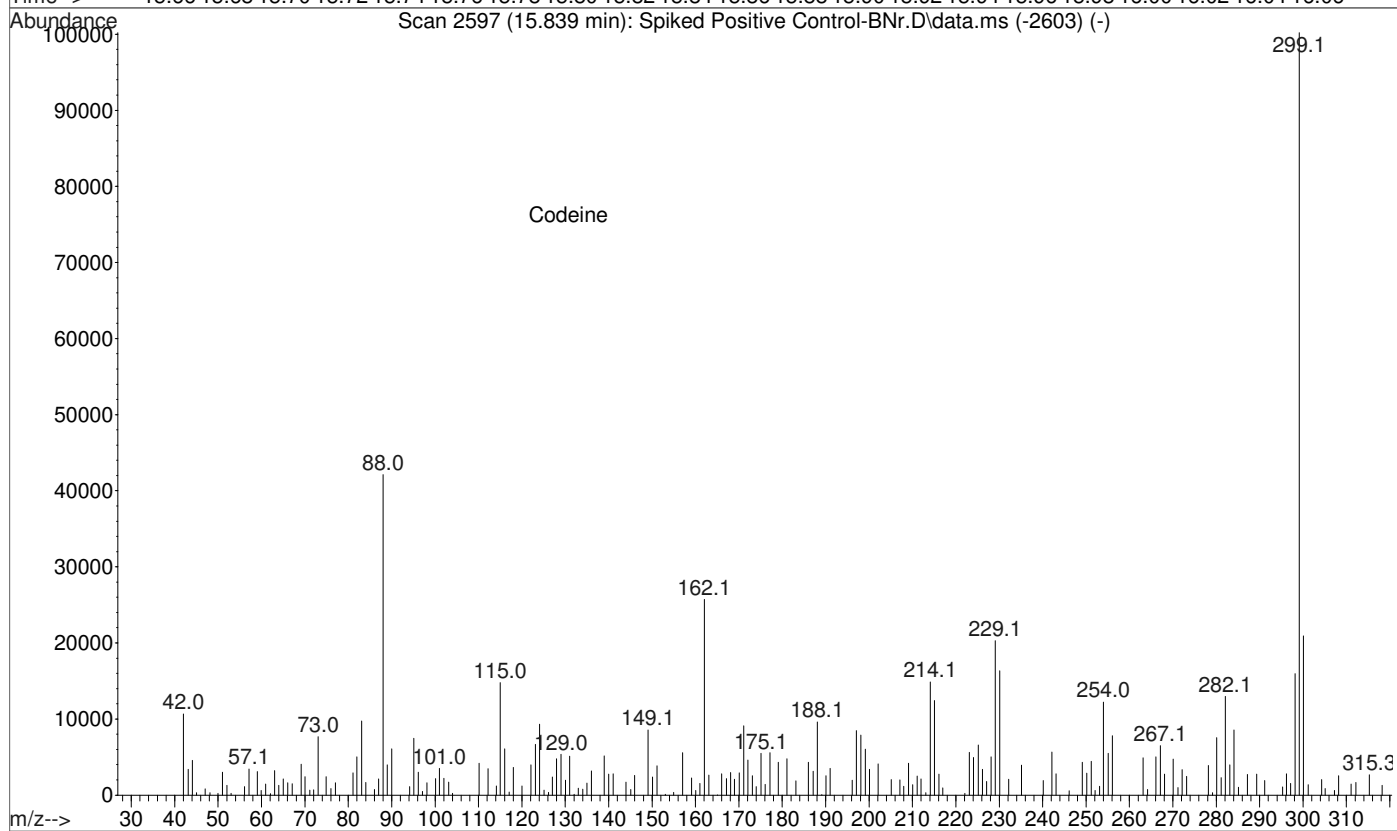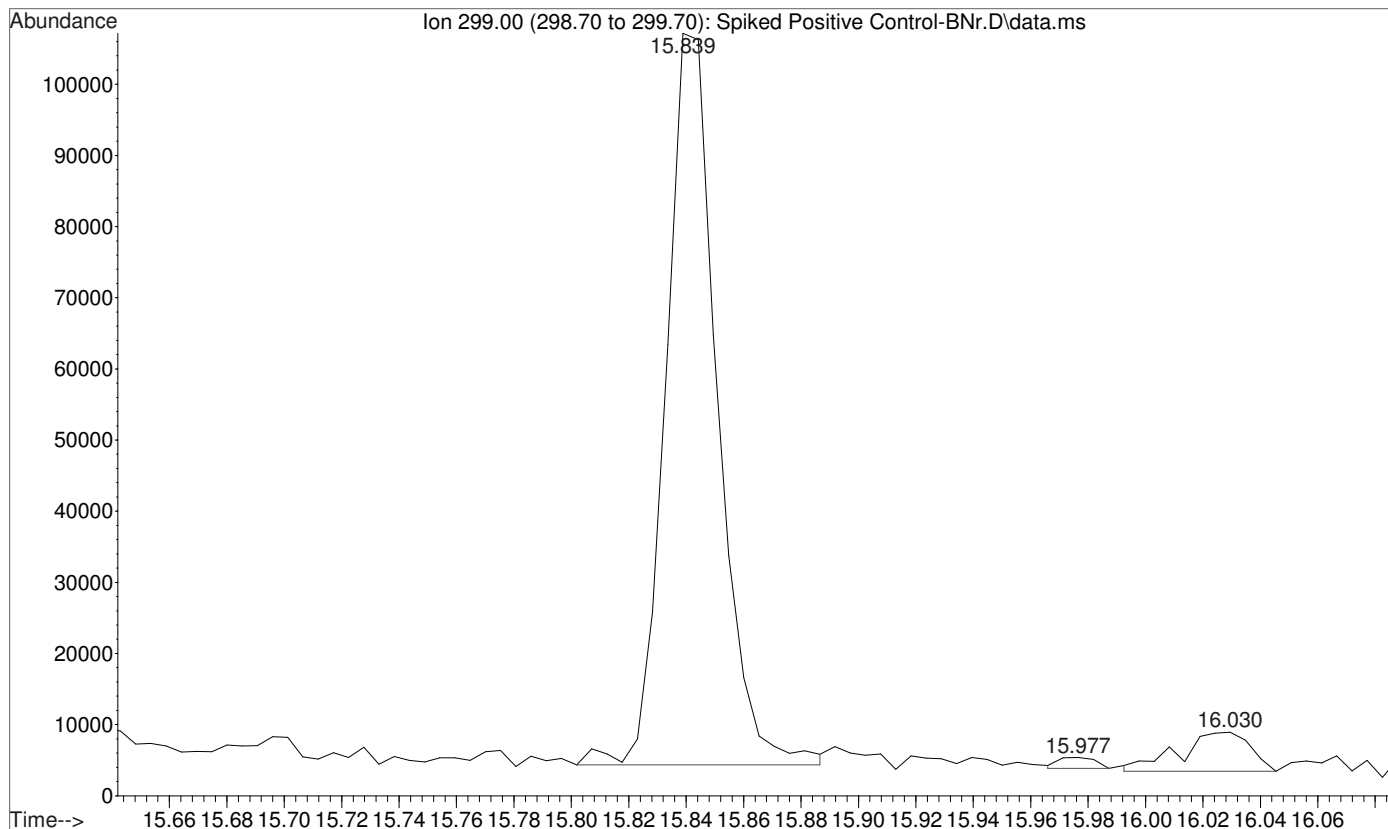



File :C:\gcms\1\data\Blood\100215\Reinjection Longer GC Method\Spi
... ked Positive Control-BNr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 03 Oct 2015 02:34 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Positive Control
Misc Info : Analytical Method 3.6.1

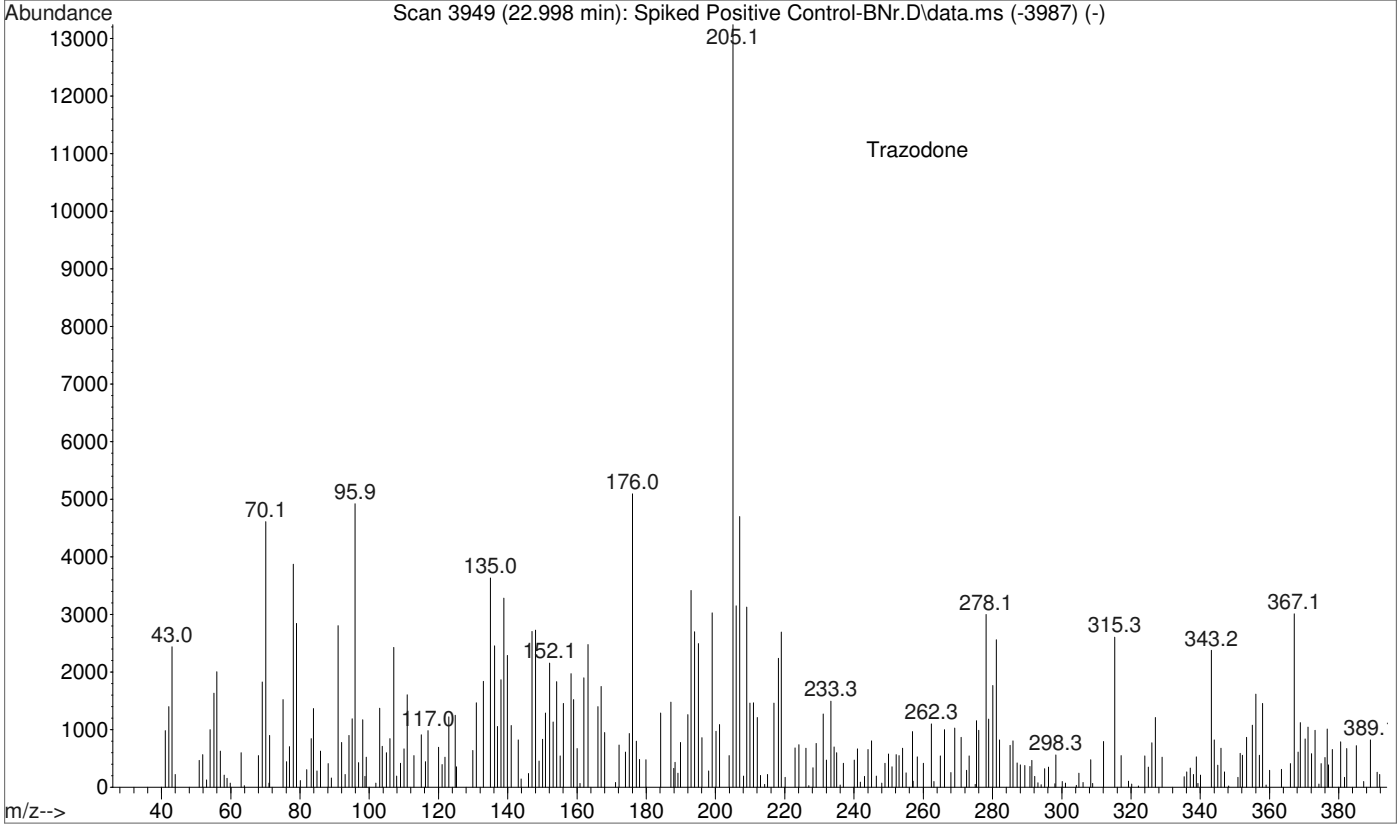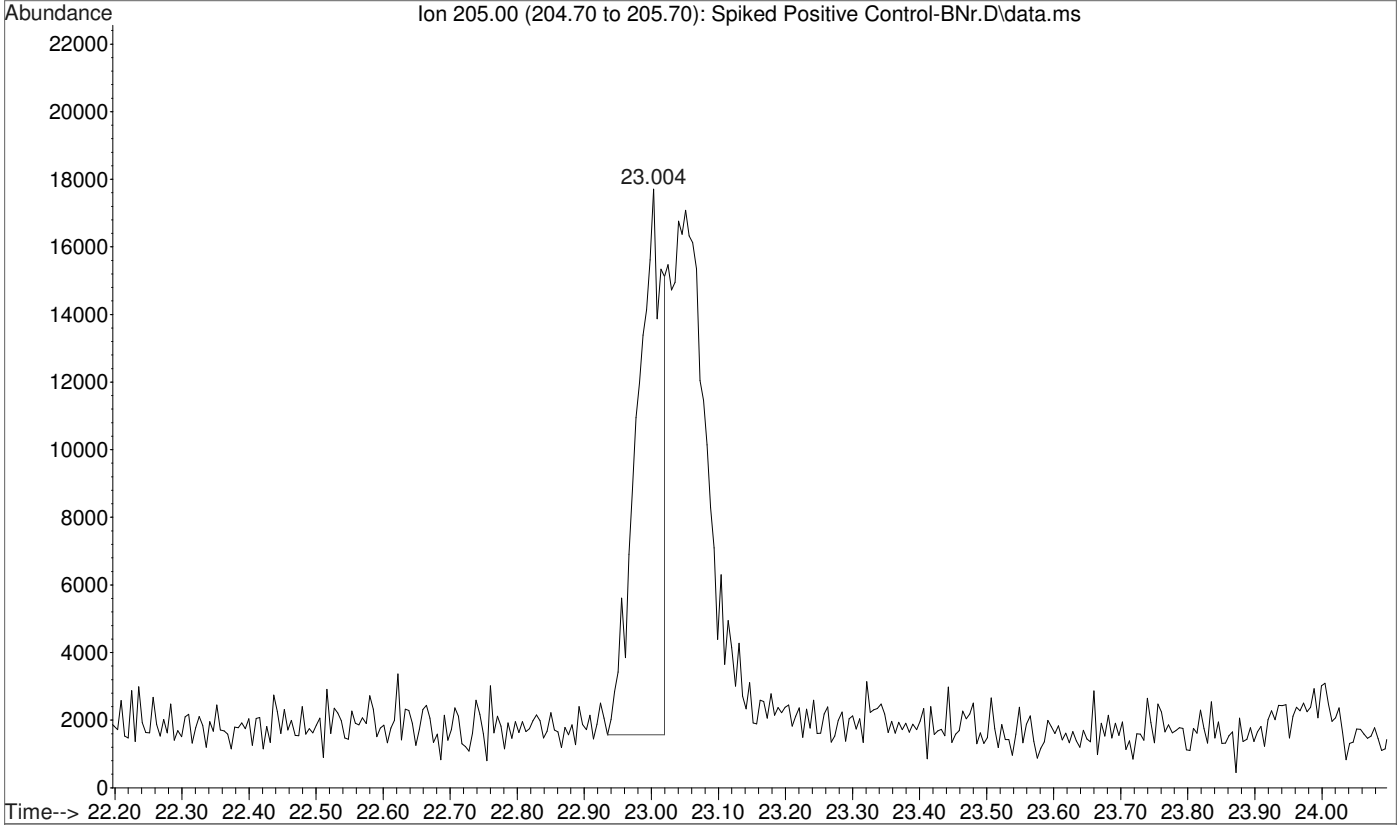

File :C:\gcms\1\data\Blood\100215\Reinjection Longer GC Method\prb
... LK2r.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 03 Oct 2015 03:08 using AcqMethod GBT092509-Delta EMV.M
Sample Name: Solvent Blank
Misc Info : Chloroform

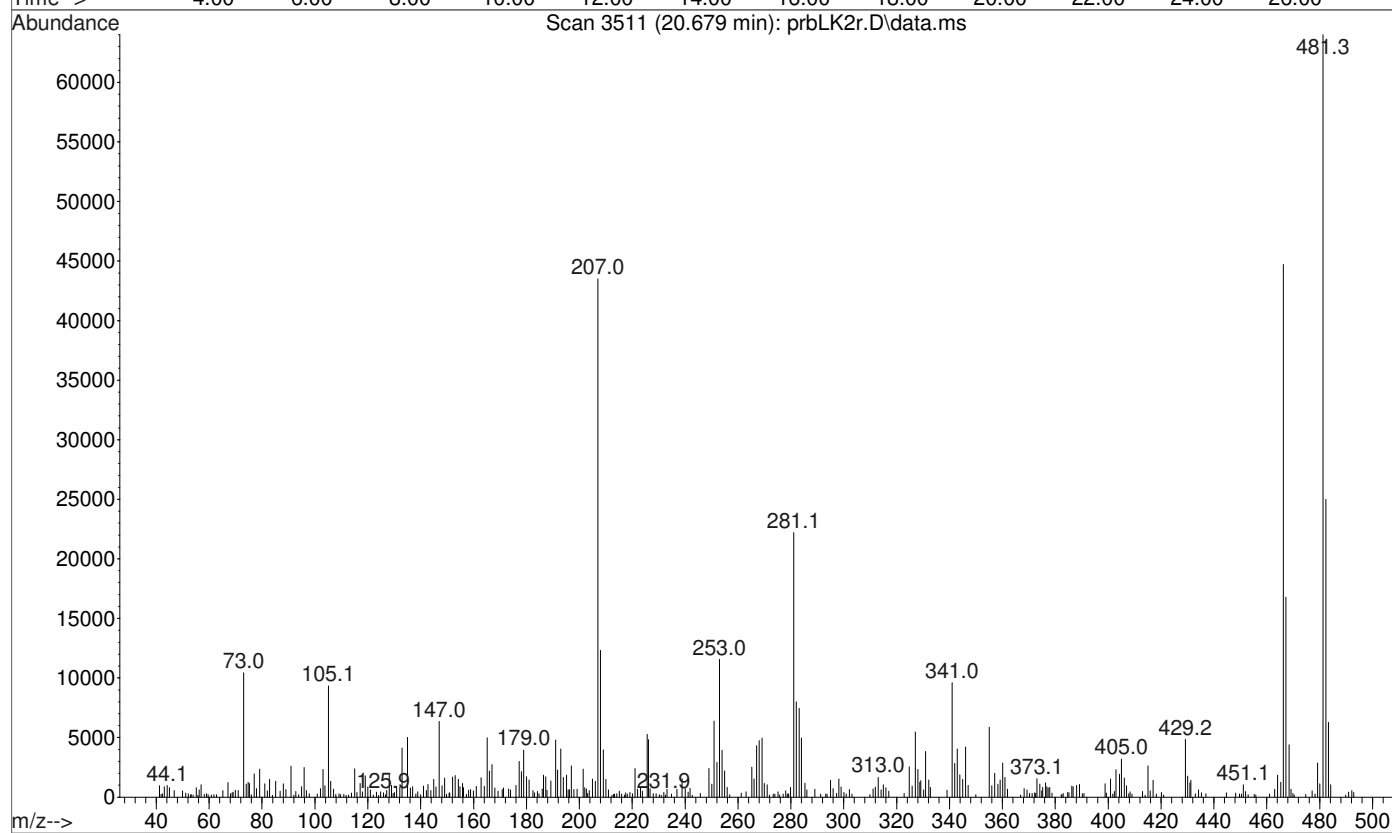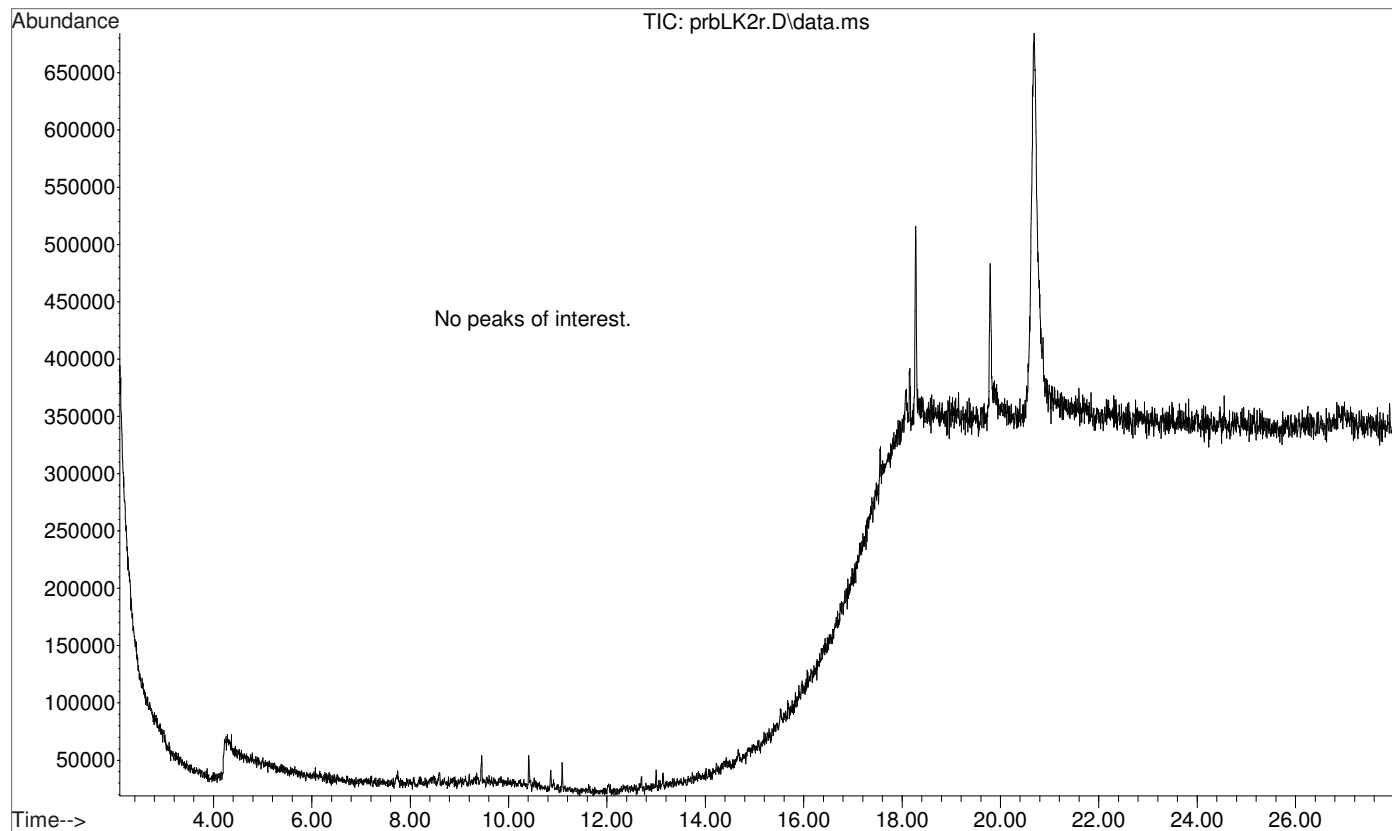

File :C:\gcms\1\data\Blood\100215\Reinjection Longer GC Method\POS
... TBLKr.D
Operator : ISP\datastor
Instrument : Major Mass Spec
Acquired : 06 Oct 2015 09:39 using AcqMethod BNSB120510.M
Sample Name: BLK
Misc Info : Chloroform

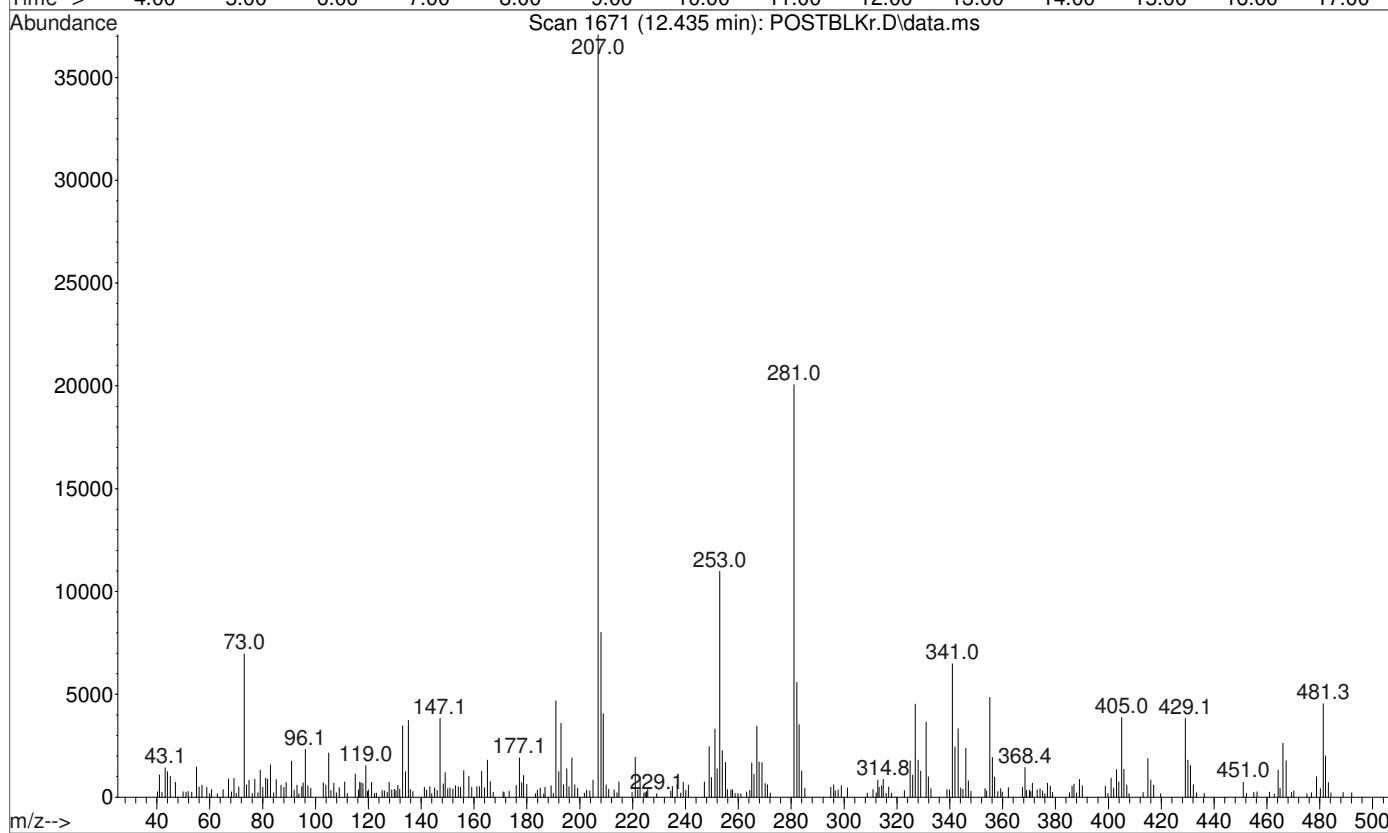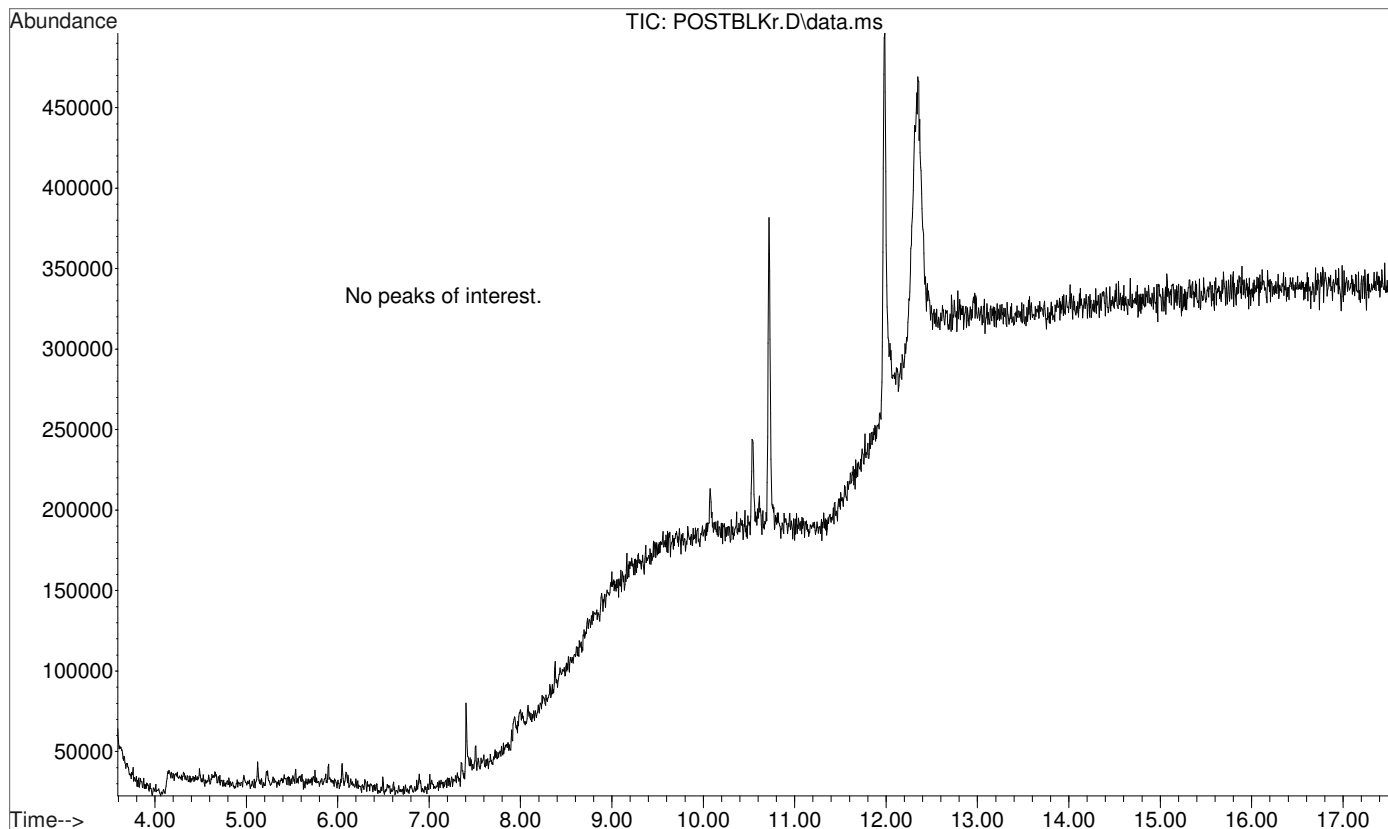

File :C:\gcms\1\data\Blood\100215\AFTER.D
Operator : ISP\datastor
Acquired : 06 Oct 2015 10:02 using AcqMethod GBT092509-Delta EMV.M
Instrument : Major Mass Spec
Sample Name: BLK
Misc Info : Chloroform
Vial Number: 56

