

REVIEWED


By Melissa (Nikka) Bradley at 10:02 am, Feb 12, 2025

NB

1/21/2025

Worklist: 7025

LAB CASE	ITEM	ITEM TYPE	DESCRIPTION
P2025-0069	1	BCK	Alcohol Analysis
P2025-0078	1	BCK	Alcohol Analysis
P2025-0079	1	BCK	Alcohol Analysis
P2025-0080	1	BCK	Alcohol Analysis
P2025-0083	1	BCK	Alcohol Analysis
P2025-0084	1	BCK	Alcohol Analysis
P2025-0091	2	BCK	Alcohol Analysis
P2025-0097	1	BCK	Alcohol Analysis
P2025-0098	1	BCK	Alcohol Analysis
P2025-0112	1	BCK	Alcohol Analysis
P2025-0114	1	BCK	Alcohol Analysis
P2025-0124	1	BCK	Alcohol Analysis
P2025-0134	1	BCK	Alcohol Analysis
P2025-0136	1	BCK	Alcohol Analysis
P2025-0149	1	BCK	Alcohol Analysis
P2025-0155	1	BCK	Alcohol Analysis
P2025-0156	1	BCK	Alcohol Analysis
P2025-0158	1	BCK	Alcohol Analysis
P2025-0159	1	BCK	Alcohol Analysis
P2025-0167	1	BCK	Alcohol Analysis
P2025-0168	1	BCK	Alcohol Analysis

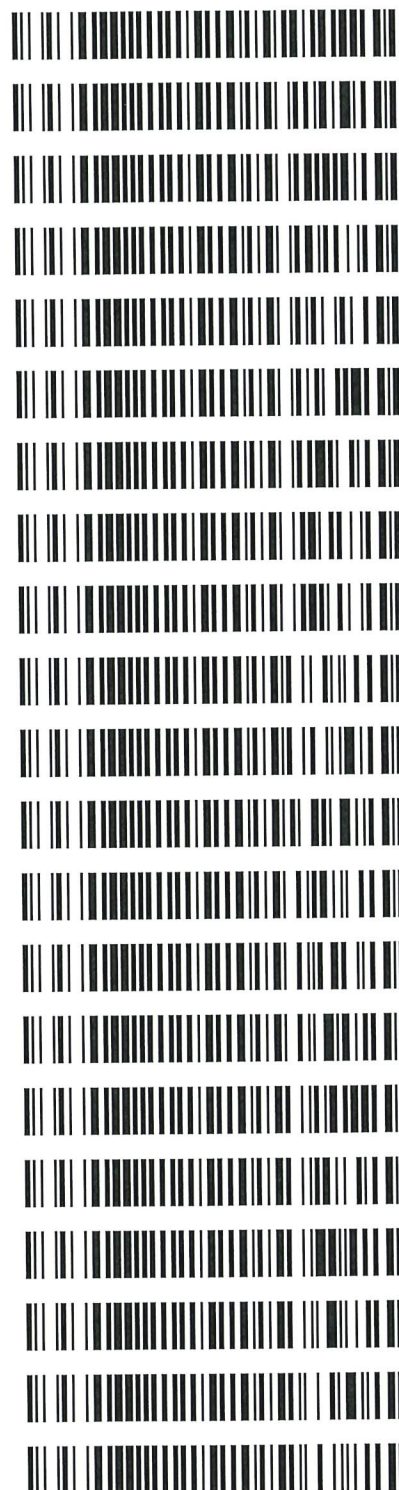

* Samples originally sampled on 01-20-25 but were not run due to contamination in the internal standard solution. The cases were re-sampled and ran on 02-07-25.

2-11-25 TS

TS

Worklist: 7025

<u>LAB CASE</u>	<u>ITEM</u>	<u>ITEM TYPE</u>	<u>DESCRIPTION</u>
P2025-0185	1	BCK	Alcohol Analysis
P2025-0187	1	BCK	Alcohol Analysis



TS

Quantitative Analysis for Ethanol & Qualitative Analysis for Other Volatiles

Analytical Method(s): 1.0

Device: Hamilton MICROLAB Liquid Processor/Dilutor Serial Number: ML600GB9897

Volatiles Quality Assurance Controls

Run Date(s): 02/07/2025

Calibration Date: (if different)

Worklist #:

7025

Control level	Expiration	Lot #		Target Value	Acceptable Range	Overall Results	
Level 1	Oct-26	2209047		0.0877	0.0789-0.0964	0.0807 g/100cc	
						0.0868 g/100cc	
						g/100cc	
Level 2	Mar-26	2110181		0.2030	0.1827-0.2233	0.2070 g/100cc	
						0.2159 g/100cc	
						g/100cc	
Multi-Component mixture:		Exp:	2028 May	Lot #	FN02162310		
Curve Fit:				Column 1	0.99997	Column2	0.99996

0.2073
NB 2/12/25

Ethanol Calibration Reference Material

Calibrator level	Target Value	Acceptable Range	Column 1	Column 2	Precision	Mean
50	0.050	0.045 - 0.055	0.0507	0.0510	0.0003	0.0508
100	0.100	0.090 - 0.110	0.1003	0.1001	0.0002	0.1002
200	0.200	0.180 - 0.220	0.1988	0.1986	0.0002	0.1987
300	0.300	0.270 - 0.330	0.2993	0.2993	0	0.2993
400	0.400	0.360 - 0.440			0	#DIV/0!
500	0.500	0.450 - 0.550	0.5006	0.5008	0.0002	0.5007

Aqueous Controls

Control level	Target Value	Acceptable Range	Overall Results
80	0.080	0.076 - 0.084	0.081 g/100cc

Internal Standard Monitoring Worksheet

Worklist #:	7025	Run Date(s):	02/07/2025
-------------	------	--------------	------------

Internal Standard Solution:	Prep Date:	1/21/2025	Exp Date:	7/21/2025
-----------------------------	------------	-----------	-----------	-----------

Sample Name	Column 1 Value	Column 2 Value
0.080	195253	194038
0.080	203053	202007
QC1	205976	204874
QC1	205563	204401
QC1	215203	214582
QC1	222903	222159
QC1		
QC1		
QC2	199921	198872
QC2	201873	200768
QC2	221340	220974
QC2	219242	218956
QC2		
QC2		

	Average	(-)20%	(+)20%
Column 1	209032.7	167226.2	250839.2
Column 2	208163.1	166530.5	249795.7

Calibration Table

Laboratory: Pocatello
Instrument Name : GC SN- C12255850662 / HS SN- C12595700014

<<Data File>>
Method File :Default Project - ALCOHOL_020725_TS.gcm
Batch File :Default Project - BATCH_020725_TS.gcb
Date Acquired :2/7/2025 9:41:29 AM
Date Created :2/7/2025 9:38:03 AM
Date Modified :2/7/2025 9:47:32 AM

Not Ready


Name : METHANOL
Detector Name: FID1
Function : $f(x)=0*x+0$
R^2 value= 0
FitType: Linear
ZeroThrough: Not Through

#	Conc.	Area	Std. Conc.	Data File Name
---	-------	------	------------	----------------

Not Ready


Name : ACETALDEHYDE
Detector Name: FID1
Function : $f(x)=0*x+0$
R^2 value= 0
FitType: Linear
ZeroThrough: Not Through

#	Conc.	Area	Std. Conc.	Data File Name
---	-------	------	------------	----------------

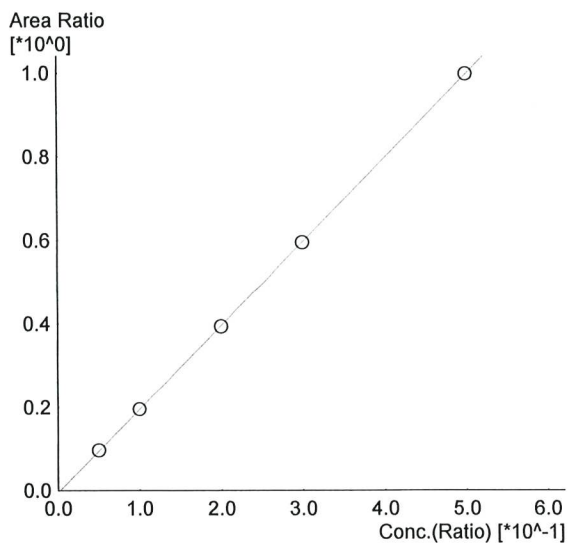


Name : ETHANOL
 Detector Name: FID1
 Function : $f(x)=2.00248*x-0.00521436$
 R² value= 0.9999781 ✓
 FitType: Linear
 ZeroThrough: Not Through

#	Conc.	Area	Std. Conc.	Data File Name
1	0.050	19366	0.0507	0.050_272025_001.gcd
2	0.100	39468	0.1003	0.100_272025_002.gcd
3	0.200	80215	0.1988	0.200_272025_003.gcd
4	0.300	121019	0.2993	0.300_272025_004.gcd
5	0.500	207850	0.5006	0.500_272025_005.gcd

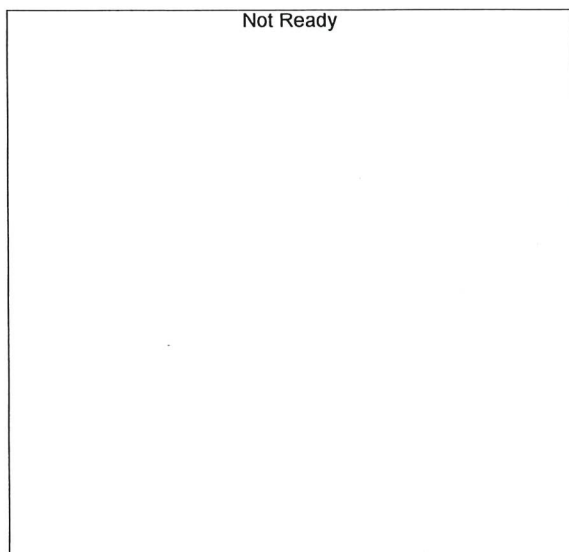

Name : ISOPROPYL ALCOHOL
 Detector Name: FID1
 Function : $f(x)=0*x+0$
 R² value= 0
 FitType: Linear
 ZeroThrough: Not Through

#	Conc.	Area	Std. Conc.	Data File Name
---	-------	------	------------	----------------

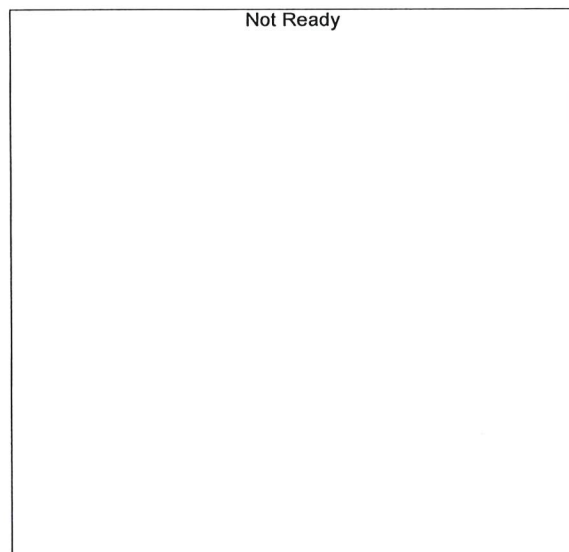

Name : ACETONE
 Detector Name: FID1
 Function : $f(x)=0*x+0$
 R² value= 0
 FitType: Linear
 ZeroThrough: Not Through

#	Conc.	Area	Std. Conc.	Data File Name
---	-------	------	------------	----------------

TS

Not Ready

Name : DFE/TFE
Detector Name: FID1
Function : $f(x)=0*x+0$
R^2 value= 0
FitType: Linear
ZeroThrough: Not Through

#	Conc.	Area	Std. Conc.	Data File Name
---	-------	------	------------	----------------

Not Ready

Name : DME
Detector Name: FID1
Function : $f(x)=0*x+0$
R^2 value= 0
FitType: Linear
ZeroThrough: Not Through


#	Conc.	Area	Std. Conc.	Data File Name
---	-------	------	------------	----------------

Not Ready

Name : ACETALDEHYDE
Detector Name: FID2
Function : $f(x)=0*x+0$
R^2 value= 0
FitType: Linear
ZeroThrough: Not Through


#	Conc.	Area	Std. Conc.	Data File Name
---	-------	------	------------	----------------

15

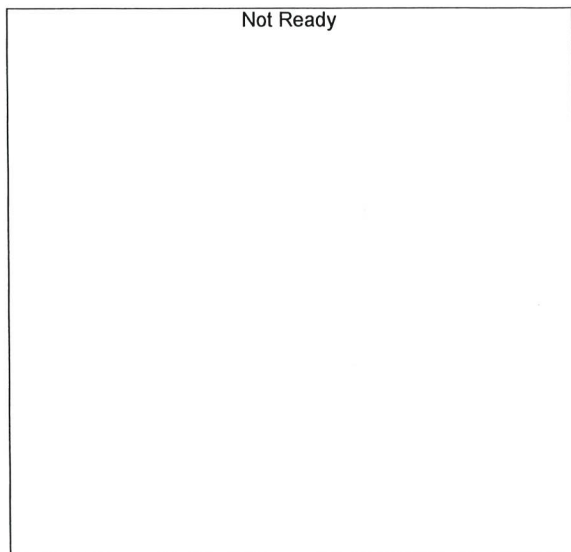


Name : METHANOL
 Detector Name: FID2
 Function : $f(x)=0*x+0$
 R^2 value= 0
 FitType: Linear
 ZeroThrough: Not Through

#	Conc.	Area	Std. Conc.	Data File Name
---	-------	------	------------	----------------

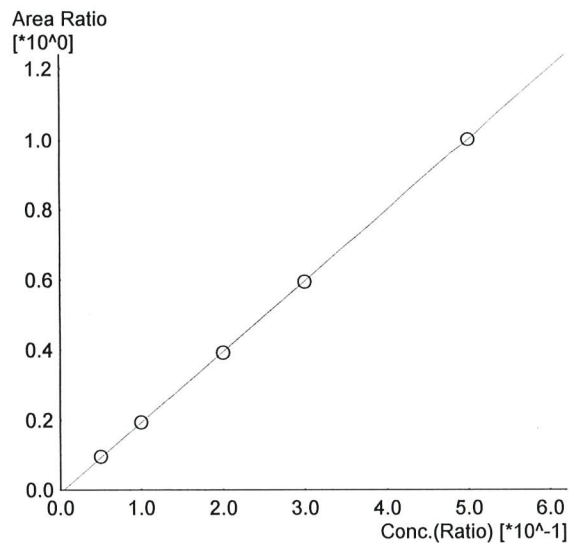

Name : ETHANOL
 Detector Name: FID2
 Function : $f(x)=2.01853*x-0.00911661$
 R^2 value= 0.9999683
 FitType: Linear
 ZeroThrough: Not Through

#	Conc.	Area	Std. Conc.	Data File Name
1	0.050	18784	0.0510	0.050_272025_001.gcd
2	0.100	38687	0.1001	0.100_272025_002.gcd
3	0.200	79601	0.1986	0.200_272025_003.gcd
4	0.300	120914	0.2993	0.300_272025_004.gcd
5	0.500	209015	0.5008	0.500_272025_005.gcd

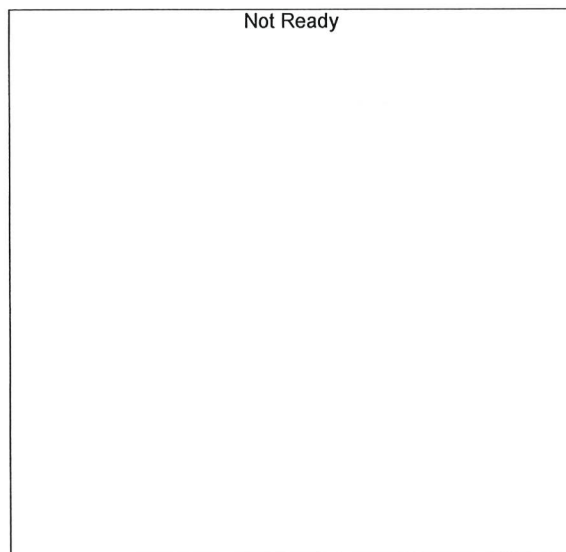

Name : ACETONE
 Detector Name: FID2
 Function : $f(x)=0*x+0$
 R^2 value= 0
 FitType: Linear
 ZeroThrough: Not Through

#	Conc.	Area	Std. Conc.	Data File Name
---	-------	------	------------	----------------

TS

Not Ready

Name : ISOPROPYL ALCOHOL
Detector Name: FID2
Function : $f(x)=0*x+0$
R^2 value= 0
FitType: Linear
ZeroThrough: Not Through

#	Conc.	Area	Std. Conc.	Data File Name
---	-------	------	------------	----------------

Not Ready

Name : DFE
Detector Name: FID2
Function : $f(x)=0*x+0$
R^2 value= 0
FitType: Linear
ZeroThrough: Not Through

#	Conc.	Area	Std. Conc.	Data File Name
---	-------	------	------------	----------------



Not Ready

Name : TFE
Detector Name: FID2
Function : $f(x)=0*x+0$
R^2 value= 0
FitType: Linear
ZeroThrough: Not Through

#	Conc.	Area	Std. Conc.	Data File Name
---	-------	------	------------	----------------

15

Sample Name : 0.050
 Vial # : 1
 Data Filename : 0.050_272025_001.gcd
 Method Filename : ALCOHOL_020725_TS.gcm
 Batch Filename : BATCH_020725_TS.gcb
 Date Acquired : 2/7/2025 9:03:24 AM
 Date Processed : 2/11/2025 12:32:28 PM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

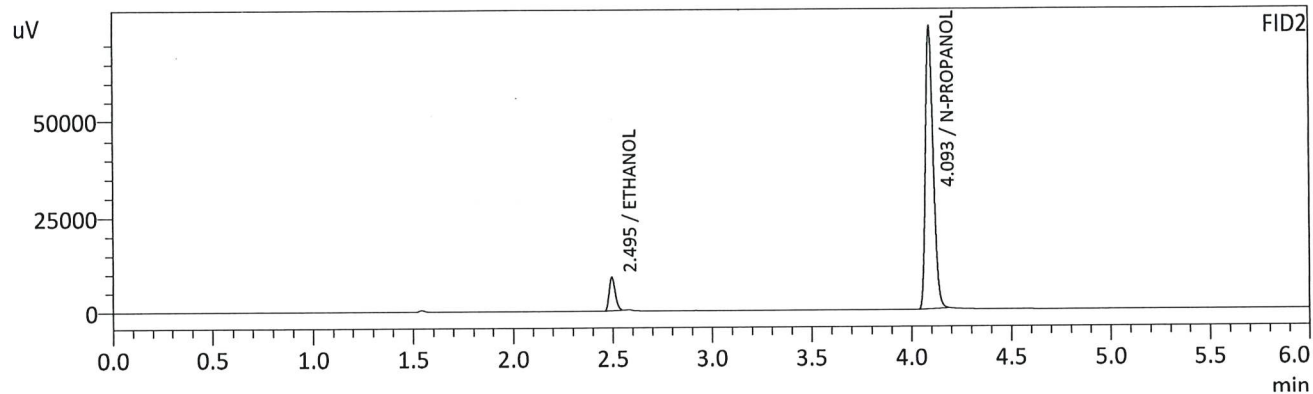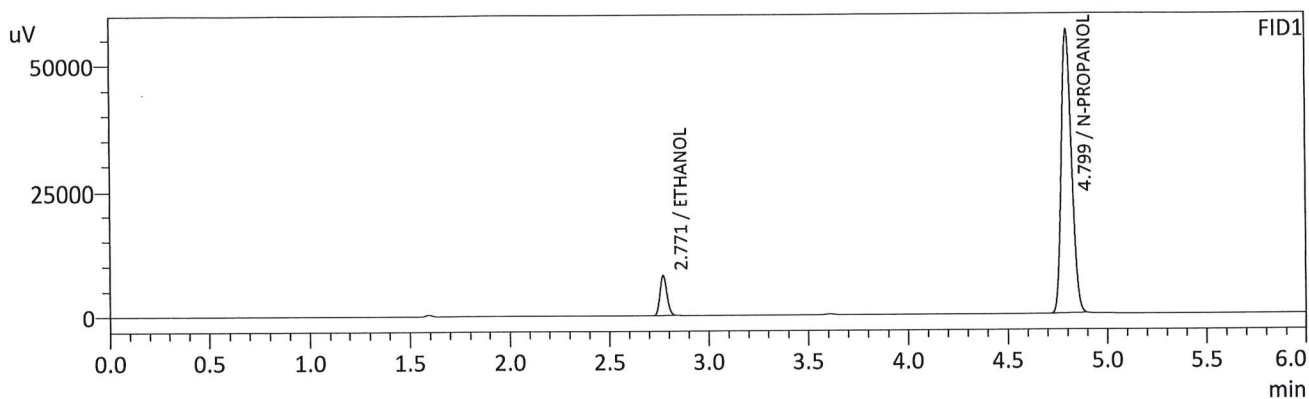

FID1



Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	0.0507	g/100cc	19366	7978
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	200841	56290
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	0.0510	g/100cc	18784	8973
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	199888	73500
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

TS

Sample Name : 0.100
 Vial # : 2
 Data Filename : 0.100_272025_002.gcd
 Method Filename : ALCOHOL_020725_TS.gcm
 Batch Filename : BATCH_020725_TS.gcb
 Date Acquired : 2/7/2025 9:12:54 AM
 Date Processed : 2/11/2025 12:32:32 PM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

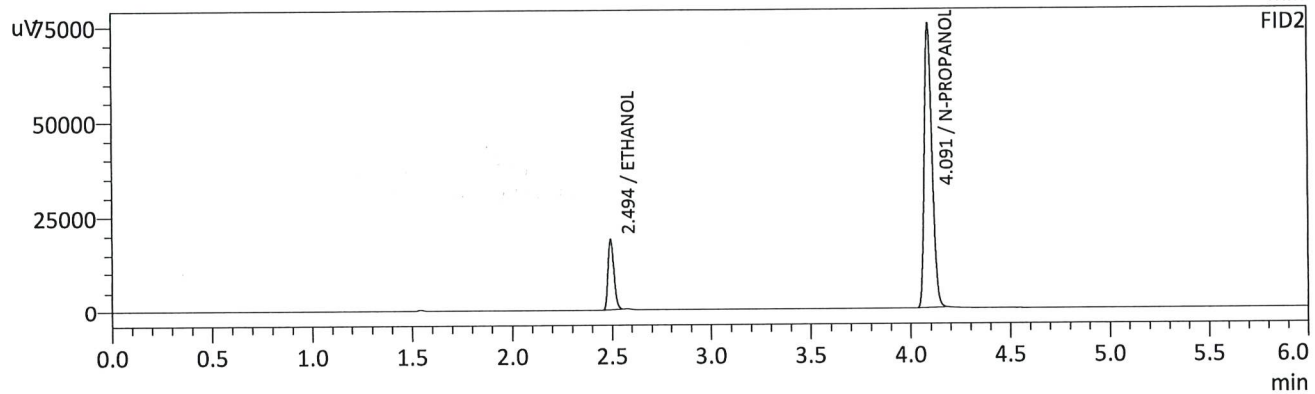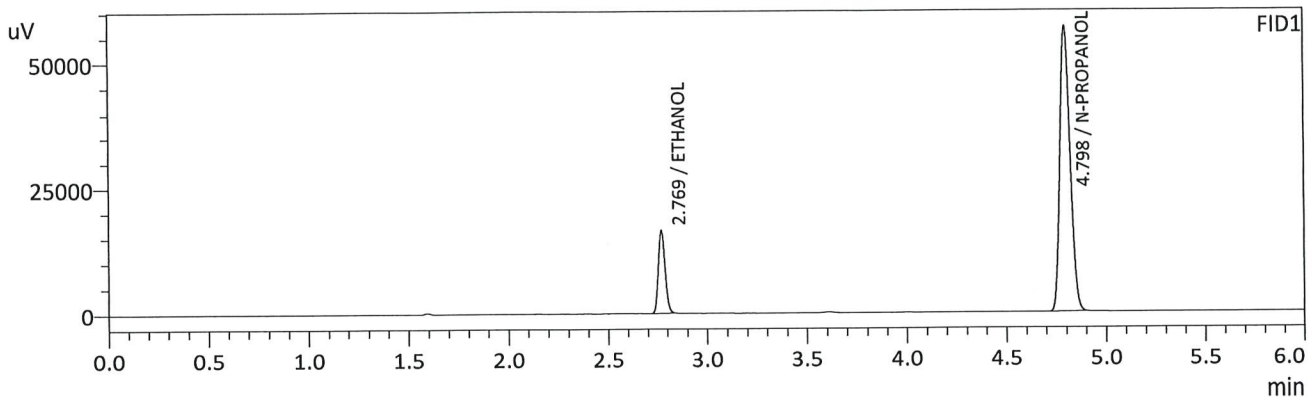

FID1


Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	0.1003	g/100cc	39468	16324
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	201731	56567
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	0.1001	g/100cc	38687	18679
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	200441	74843
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

B

Sample Name : 0.200
 Vial # : 3
 Data Filename : 0.200_272025_003.gcd
 Method Filename : ALCOHOL_020725_TS.gcm
 Batch Filename : BATCH_020725_TS.gcb
 Date Acquired : 2/7/2025 9:22:14 AM
 Date Processed : 2/11/2025 12:32:35 PM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

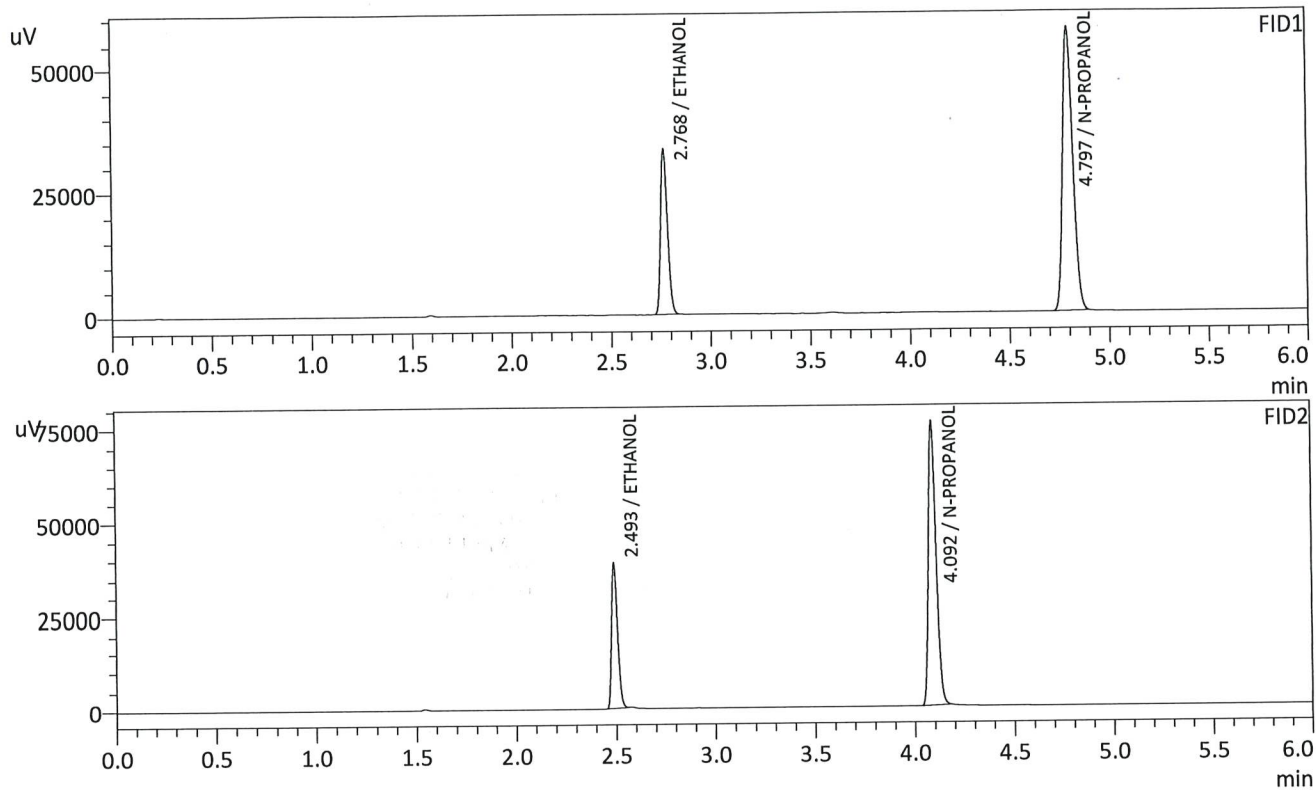

FID1


Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	0.1988	g/100cc	80215	33044
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	204079	57240
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	0.1986	g/100cc	79601	38271
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	203118	75618
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

AS

Sample Name : 0.300
 Vial # : 4
 Data Filename : 0.300_272025_004.gcd
 Method Filename : ALCOHOL_020725_TS.gcm
 Batch Filename : BATCH_020725_TS.gcb
 Date Acquired : 2/7/2025 9:32:00 AM
 Date Processed : 2/11/2025 12:32:39 PM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

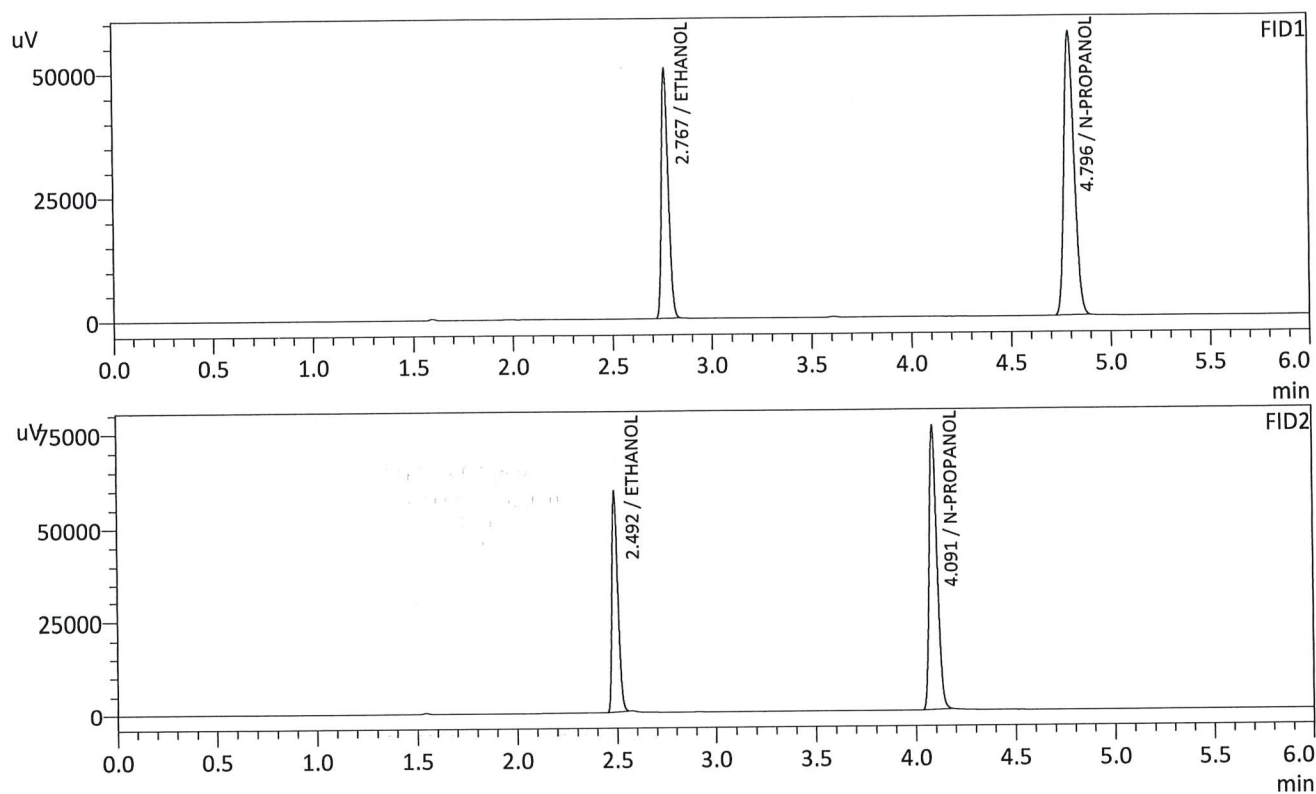

FID1



Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	0.2993	g/100cc	121019	50113
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	203655	57220
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	0.2993	g/100cc	120914	58582
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	203191	75813
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

TS

Sample Name : 0.500
 Vial # : 5
 Data Filename : 0.500_272025_005.gcd
 Method Filename : ALCOHOL_020725_TS.gcm
 Batch Filename : BATCH_020725_TS.gcb
 Date Acquired : 2/7/2025 9:41:29 AM
 Date Processed : 2/7/2025 9:47:32 AM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

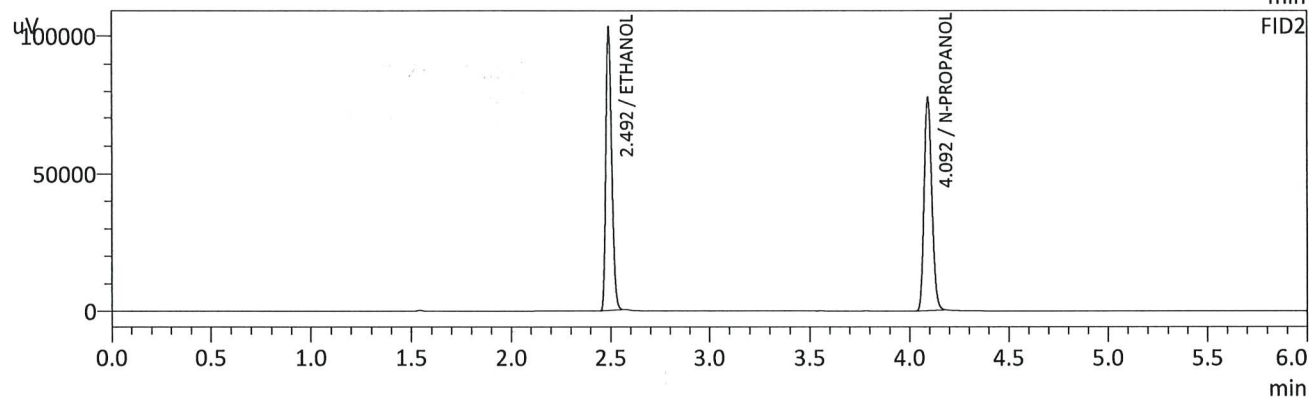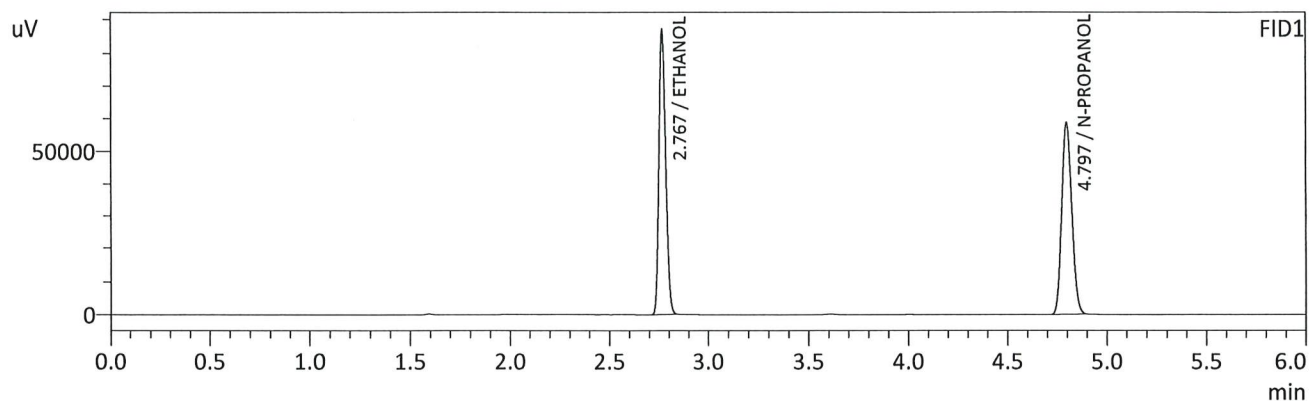

FID1



Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	0.5006	g/100cc	207850	86594
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	208388	58503
DCE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	0.5008	g/100cc	209015	102050
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	208644	77144
DCE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

TS

Sample Name : INT STD BLK 1
 Vial # : 6
 Data Filename : INT STD BLK 1_272025_006.gcd
 Method Filename : ALCOHOL_020725_TS.gcm
 Batch Filename : BATCH_020725_TS.gcb
 Date Acquired : 2/7/2025 9:50:48 AM
 Date Processed : 2/7/2025 9:56:48 AM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

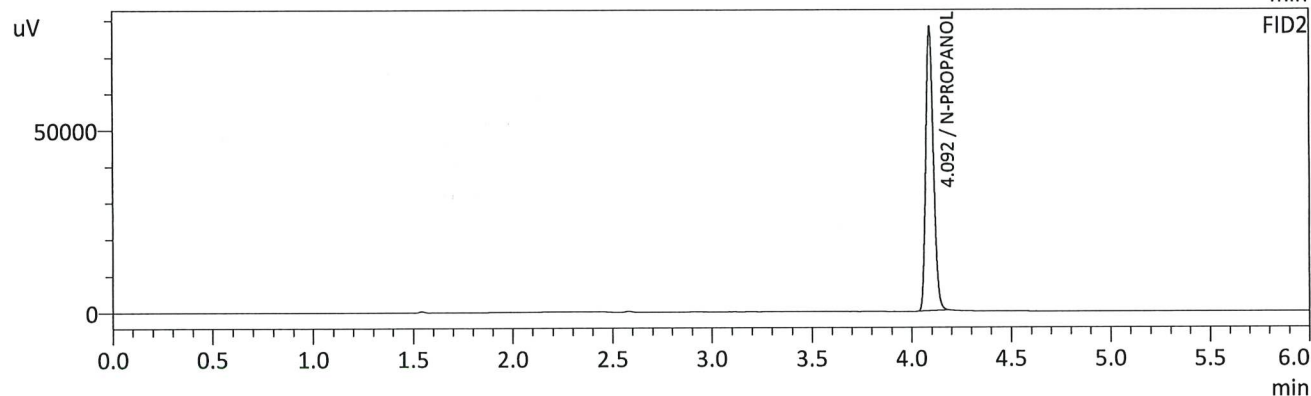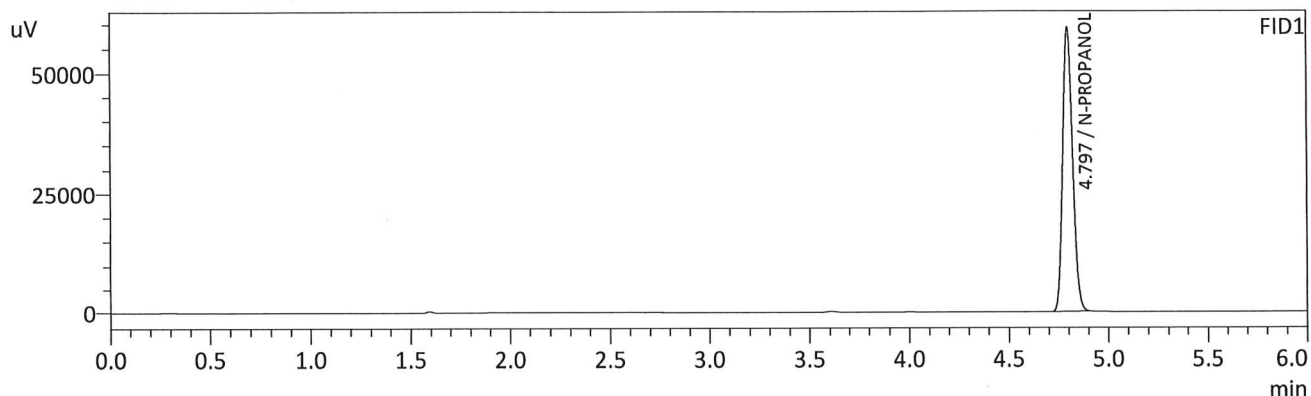

FID1


Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	209615	59041
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	208344	77747
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

13

Sample Name : MULTI-COMP MIX
 Vial # : 7
 Data Filename : MULTI-COMP MIX_272025_001.gcd
 Method Filename : ALCOHOL_020725_TS.gcm
 Batch Filename : BATCH_020725_TS.gcb
 Date Acquired : 2/7/2025 10:40:19 AM
 Date Processed : 2/7/2025 10:46:21 AM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

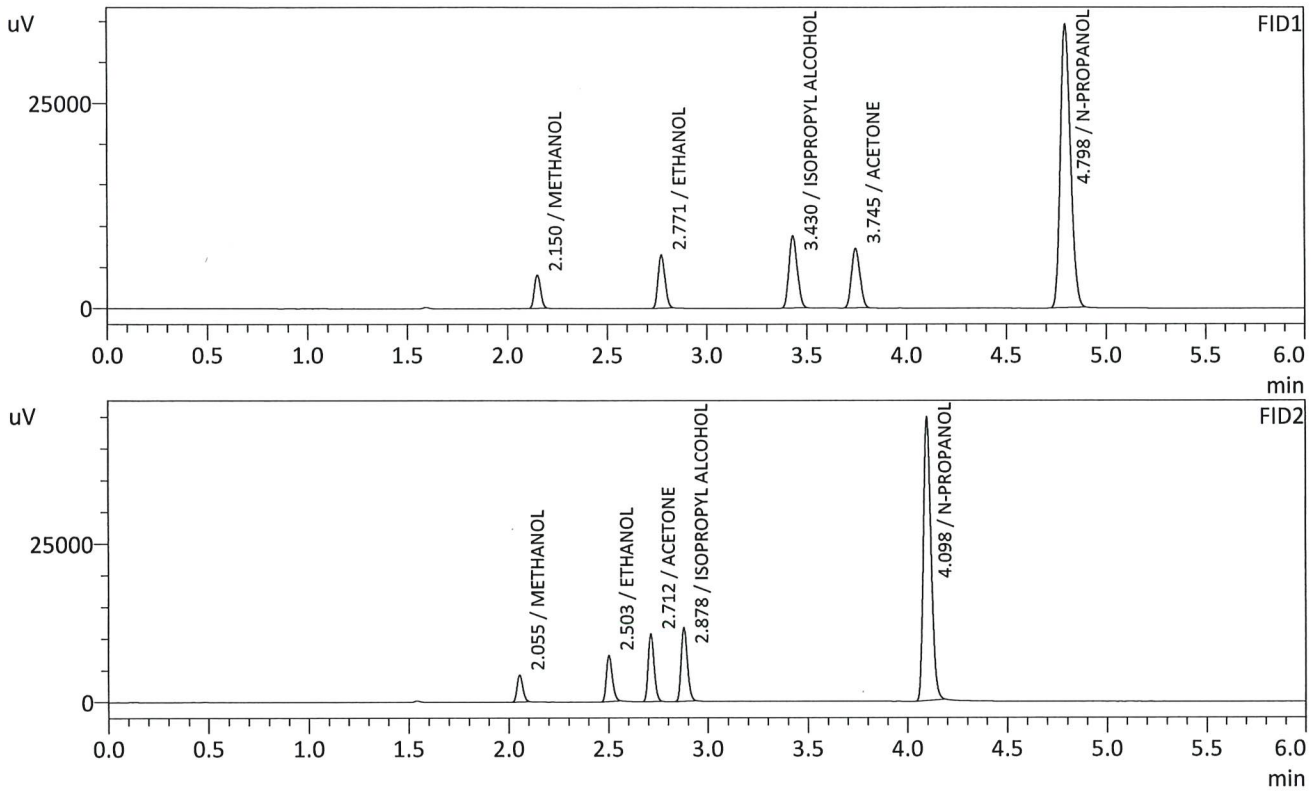

FID1



Name	Conc.	Unit	Area	Height
METHANOL	0.0000	g/100cc	8443	3897
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	0.0665	g/100cc	15579	6455
ISOPROPYL ALCOHOL	0.0000	g/100cc	24947	8715
ACETONE	0.0000	g/100cc	21090	7260
N-PROPANOL	0.0000	g/100cc	121575	34467
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	0.0000	g/100cc	8473	4203
ETHANOL	0.0672	g/100cc	15127	7214
ACETONE	0.0000	g/100cc	21916	10512
ISOPROPYL ALCOHOL	0.0000	g/100cc	25139	11560
N-PROPANOL	0.0000	g/100cc	119366	44443
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

TS

Sample Name : INT STD BLK 2
 Vial # : 8
 Data Filename : INT STD BLK 2_272025_002.gcd
 Method Filename : ALCOHOL_020725_TS.gcm
 Batch Filename : BATCH_020725_TS.gcb
 Date Acquired : 2/7/2025 10:49:49 AM
 Date Processed : 2/7/2025 10:55:50 AM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

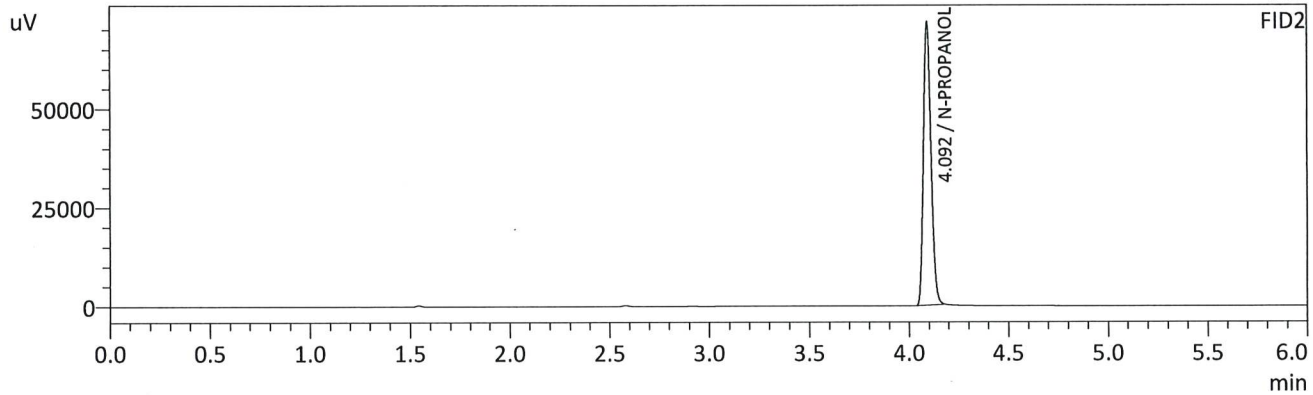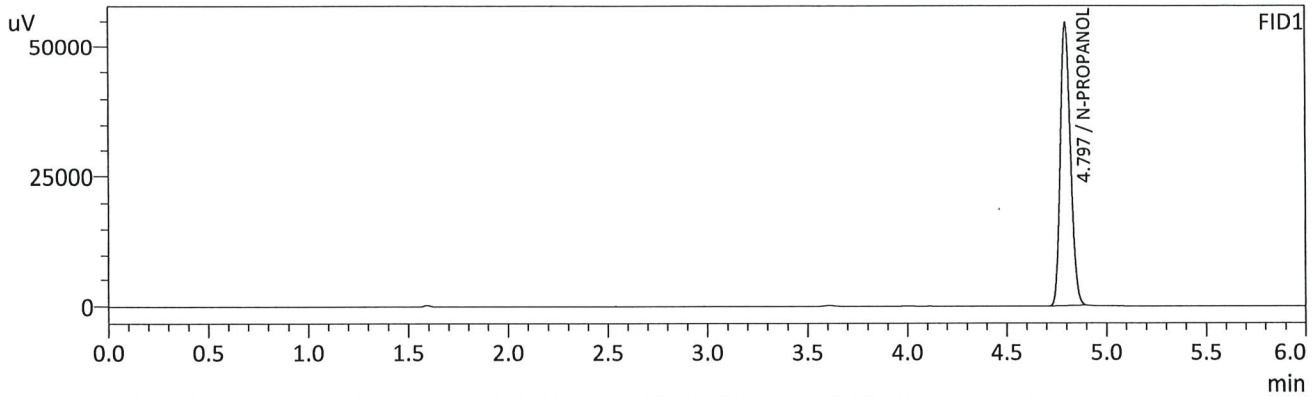

FID1

Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	193801	54551
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	192034	71409
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

VOLATILES DETERMINATION CASEFILE WORKSHEET

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No: 0.08 QA			Analysis Date(s): 2/7/2025 11:18:26 AM(-07:00)			
	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Sample A-B Difference	Over-all Mean
Sample Results	0.0829	0.0827	0.0002	0.0828	0.0020	0.0818
(g/100cc)	0.0810	0.0806	0.0004	0.0808		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument information is stored centrally.

Refer To Instrument Method: ALCOHOL_020725_TS.gcm


Reporting of Results	Uncertainty of Measurements (UM%):		5.00%
Overall Mean (g/100cc)	Low	High	5 % of Mean
0.081	0.076	0.086	0.005

	Reported Results	
	0.081	

Calibration and control data are stored centrally.

TS

Sample Name : 0.08 QA
 Vial # : 11
 Data Filename : 0.08 QA_272025_005.gcd
 Method Filename : ALCOHOL_020725_TS.gcm
 Batch Filename : BATCH_020725_TS.gcb
 Date Acquired : 2/7/2025 11:18:26 AM
 Date Processed : 2/7/2025 11:24:26 AM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

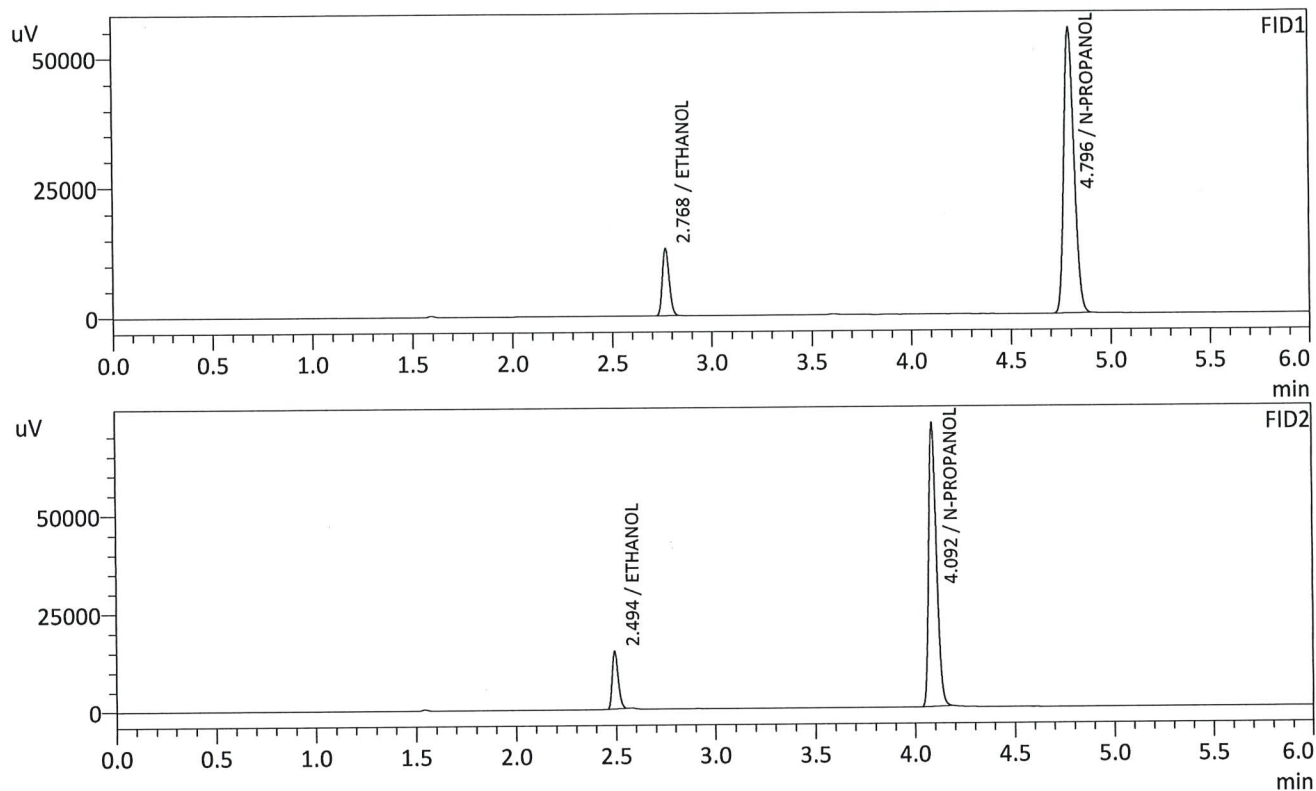

FID1



Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	0.0829	g/100cc	31431	12937
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	195253	55075
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	0.0827	g/100cc	30659	14779
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	194038	72087
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

TS

Sample Name : 0.08 QA - B
 Vial # : 12
 Data Filename : 0.08 QA - B_272025_006.gcd
 Method Filename : ALCOHOL_020725_TS.gcm
 Batch Filename : BATCH_020725_TS.gcb
 Date Acquired : 2/7/2025 11:27:43 AM
 Date Processed : 2/7/2025 11:33:45 AM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

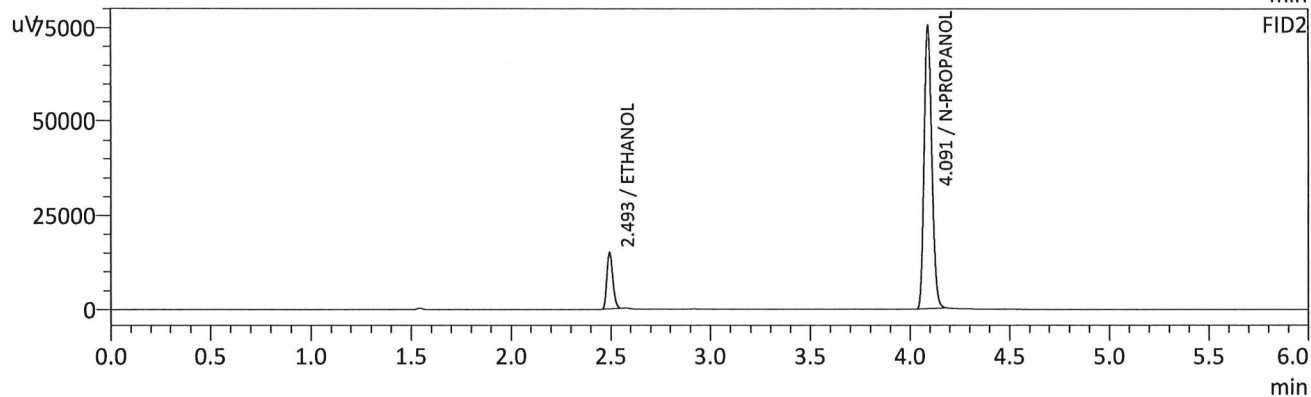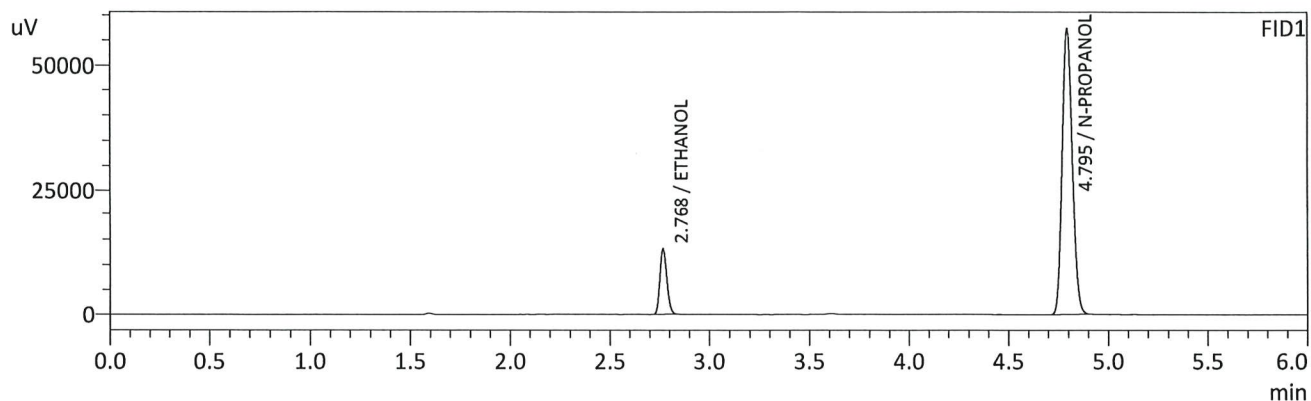

FID1

Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	0.0810	g/100cc	31881	13093
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	203053	57261
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	0.0806	g/100cc	31048	14941
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	202007	75406
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

B

VOLATILES DETERMINATION CASEFILE WORKSHEET

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No: QC1-1			Analysis Date(s): 2/7/2025 10:59:09 AM(-07:00)			
	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Sample A-B Difference	Over-all Mean
Sample Results	0.0808	0.0806	0.0002	0.0807	0.0000	0.0807
(g/100cc)	0.0808	0.0806	0.0002	0.0807		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument information is stored centrally.

Refer To Instrument Method: ALCOHOL_020725_TS.gcm


Reporting of Results	Uncertainty of Measurements (UM%): 5.00%		
Overall Mean (g/100cc)	Low	High	5 % of Mean
0.080	0.076	0.084	0.004

	Reported Results	
	0.080	

Calibration and control data are stored centrally.

TS

Sample Name : QC1-1
 Vial # : 9
 Data Filename : QC1-1_272025_003.gcd
 Method Filename : ALCOHOL_020725_TS.gcm
 Batch Filename : BATCH_020725_TS.gcb
 Date Acquired : 2/7/2025 10:59:09 AM
 Date Processed : 2/7/2025 11:05:12 AM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

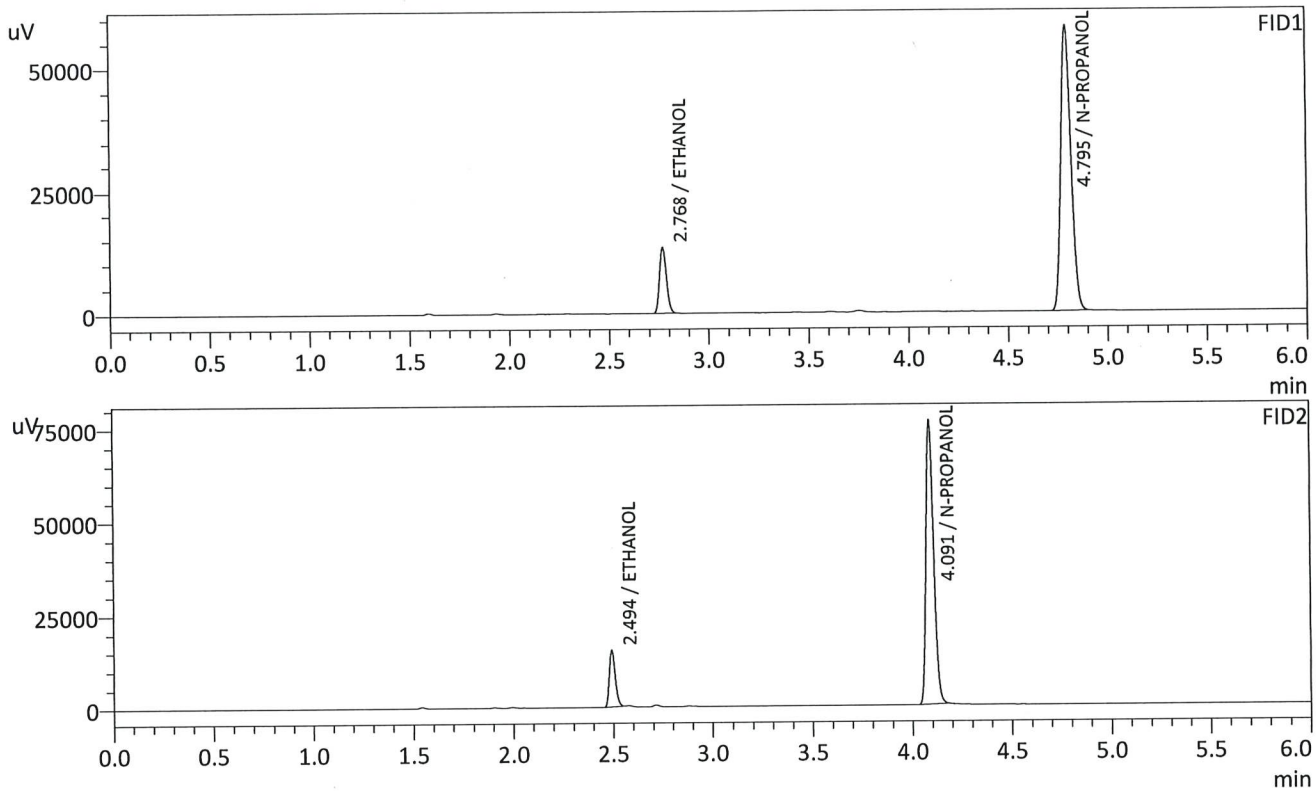

FID1



Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	0.0808	g/100cc	32269	13286
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	205976	57993
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	0.0806	g/100cc	31482	15151
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	204874	76261
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

TS

Sample Name : QC1-1-B
 Vial # : 10
 Data Filename : QC1-1-B_272025_004.gcd
 Method Filename : ALCOHOL_020725_TS.gcm
 Batch Filename : BATCH_020725_TS.gcb
 Date Acquired : 2/7/2025 11:08:54 AM
 Date Processed : 2/7/2025 11:14:56 AM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

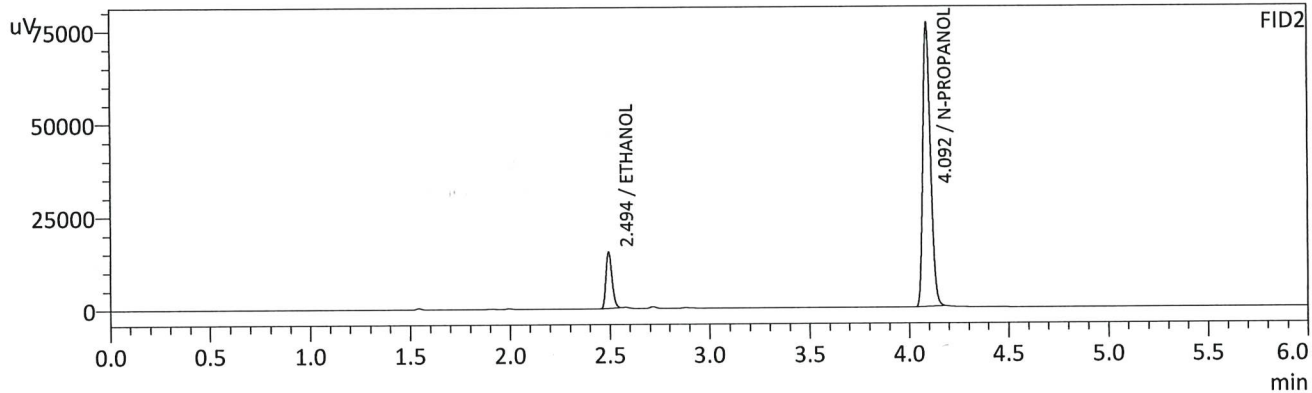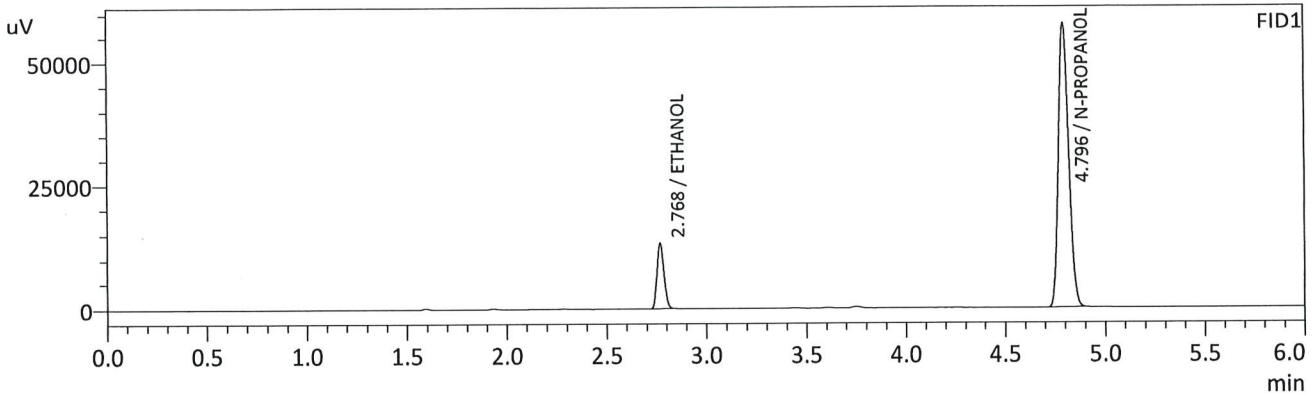

FID1

Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	0.0808	g/100cc	32224	13249
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	205563	57812
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	0.0806	g/100cc	31427	15129
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	204401	76198
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

TS

VOLATILES DETERMINATION CASEFILE WORKSHEET

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No: QC1-2				Analysis Date(s): 2/7/2025 5:58:22 PM(-07:00)		
	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Sample A-B Difference	Over-all Mean
Sample Results	0.0874	0.0867	0.0007	0.0870	0.0003	0.0868
(g/100cc)	0.0870	0.0864	0.0006	0.0867		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument information is stored centrally.

Refer To Instrument Method: ALCOHOL_020725_TS.gcm



Reporting of Results		Uncertainty of Measurements (UM%): 5.00%		
Overall Mean (g/100cc)	Low	High	5 % of Mean	
0.086	0.081	0.091	0.005	

Reported Results	
Column 1 FID A	Column 2 FID B 0.086

Calibration and control data are stored centrally.

TS

Sample Name : QC1-2
 Vial # : 53
 Data Filename : QC1-2_272025_047.gcd
 Method Filename : ALCOHOL_020725_TS.gcm
 Batch Filename : BATCH_020725_TS.gcb
 Date Acquired : 2/7/2025 5:58:22 PM
 Date Processed : 2/7/2025 6:04:24 PM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

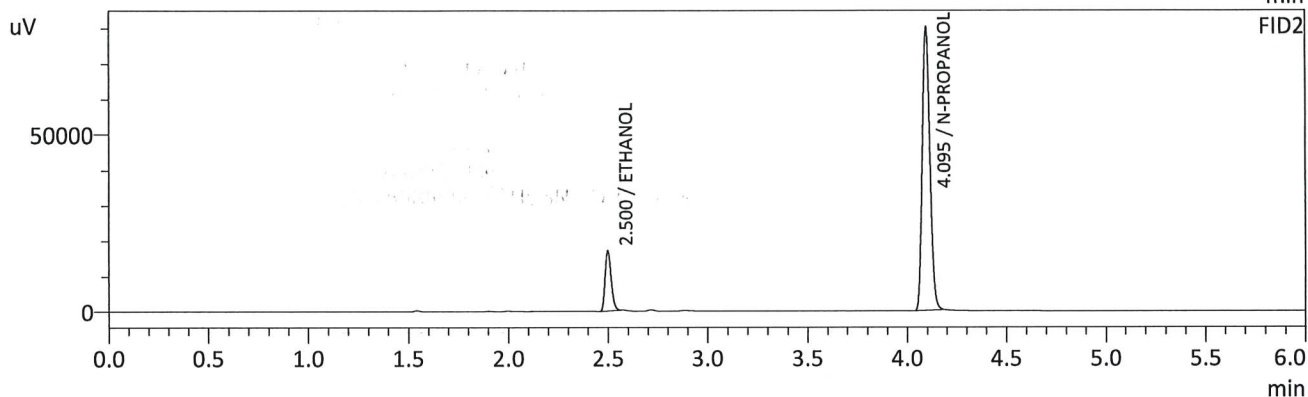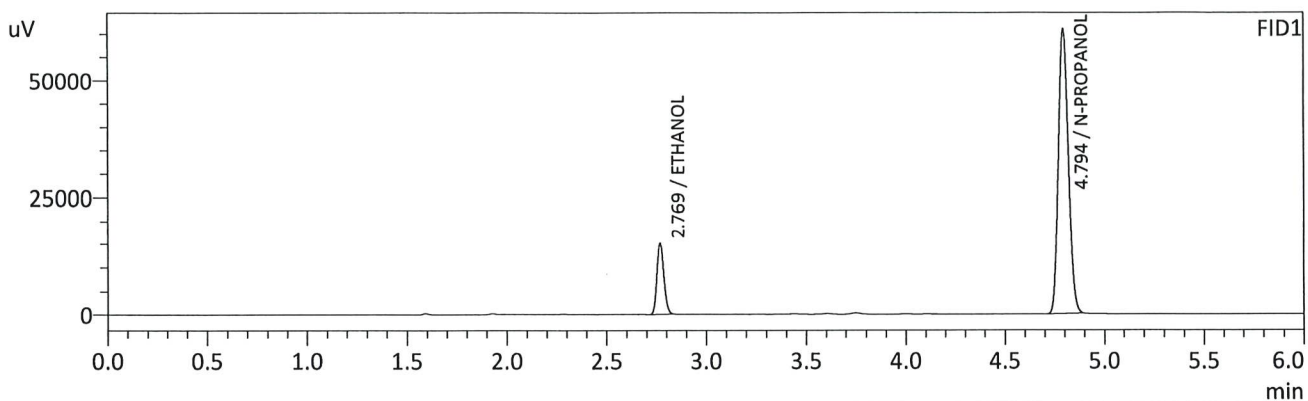

FID1



Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	0.0874	g/100cc	36546	14963
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	215203	60879
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	0.0867	g/100cc	35610	17102
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	214582	80144
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

TS

Sample Name : QC1-2-B
 Vial # : 54
 Data Filename : QC1-2-B_272025_048.gcd
 Method Filename : ALCOHOL_020725_TS.gcm
 Batch Filename : BATCH_020725_TS.gcb
 Date Acquired : 2/7/2025 6:07:40 PM
 Date Processed : 2/7/2025 6:13:42 PM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

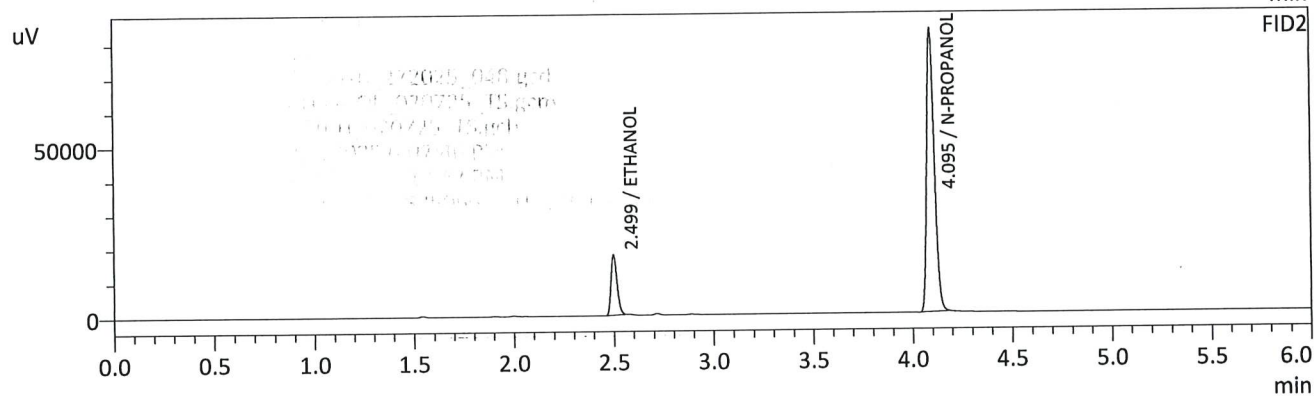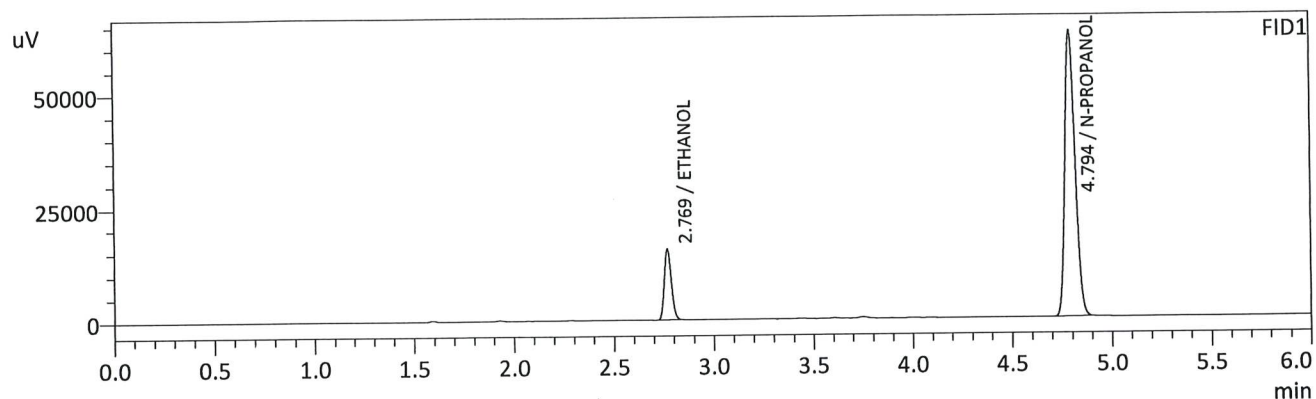

FID1

Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	0.0870	g/100cc	37671	15426
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	222903	62933
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	0.0864	g/100cc	36750	17655
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	222159	83140
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

TS

VOLATILES DETERMINATION CASEFILE WORKSHEET

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No: QC2-1

Analysis Date(s): 2/7/2025 2:28:48 PM(-07:00)

	Column 1 FID A	Column 2 FID B	Column Precision	Mean Value	Sample A-B Difference	Over-all Mean
Sample Results	0.2075	0.2073	0.0002	0.2074	0.0001	0.2073
(g/100cc)	0.2074	0.2073	0.0001	0.2073		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument information is stored centrally.

Refer To Instrument Method: ALCOHOL_020725_TS.gcm



Reporting of Results	Uncertainty of Measurements (UM%): 5.00%		
Overall Mean (g/100cc)	Low	High	5 % of Mean
0.207	0.196	0.218	0.011

	Reported Results
	0.207

Calibration and control data are stored centrally.

TS

Sample Name : QC2-1
 Vial # : 31
 Data Filename : QC2-1_272025_025.gcd
 Method Filename : ALCOHOL_020725_TS.gcm
 Batch Filename : BATCH_020725_TS.gcb
 Date Acquired : 2/7/2025 2:28:48 PM
 Date Processed : 2/7/2025 2:34:50 PM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

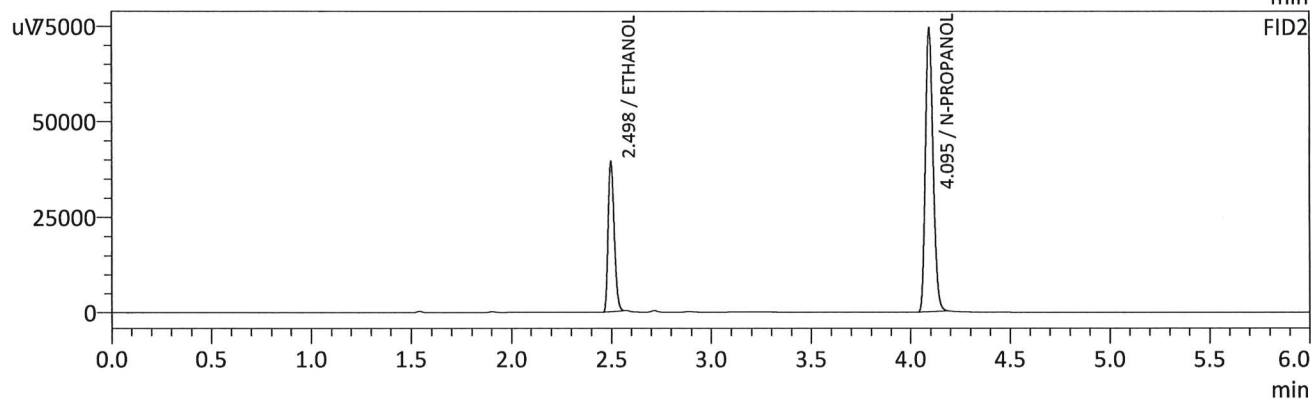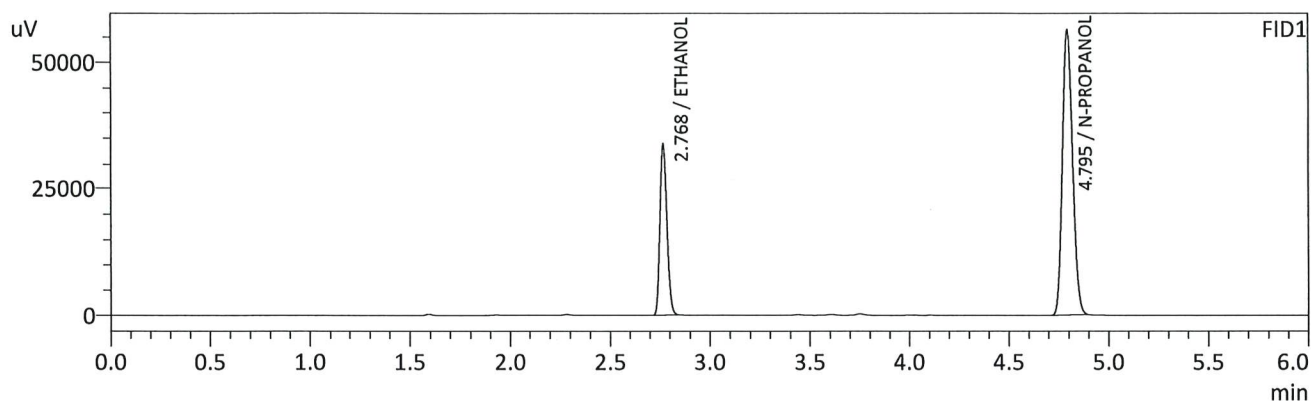

FID1



Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	0.2075	g/100cc	82056	33532
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	199921	56368
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	0.2073	g/100cc	81427	39083
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	198872	74252
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

15

Sample Name : QC2-1-B
 Vial # : 32
 Data Filename : QC2-1-B_272025_026.gcd
 Method Filename : ALCOHOL_020725_TS.gcm
 Batch Filename : BATCH_020725_TS.gcb
 Date Acquired : 2/7/2025 2:38:21 PM
 Date Processed : 2/7/2025 2:44:23 PM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

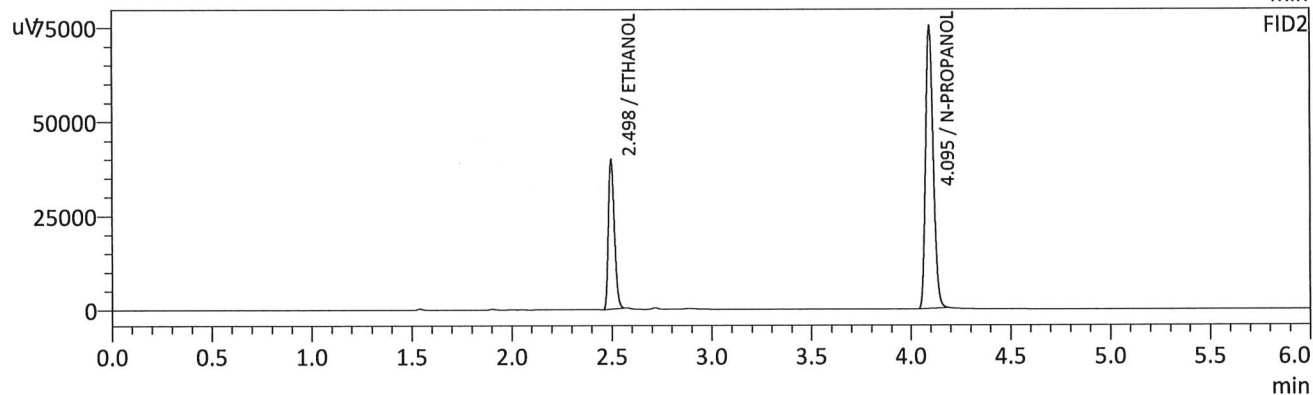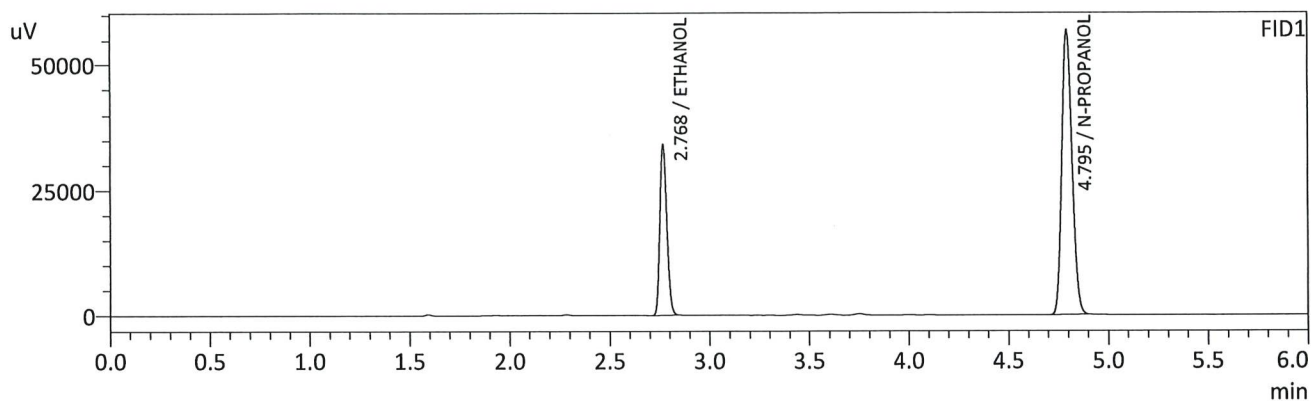

FID1

Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	0.2074	g/100cc	82791	33796
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	201873	56989
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	0.2073	g/100cc	82204	39446
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	200768	75125
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

TS

VOLATILES DETERMINATION CASEFILE WORKSHEET

VOLATILES DETERMINATION CASEFILE WORKSHEET

Laboratory No: QC2-2			Analysis Date(s): 2/7/2025 7:33:20 PM(-07:00)			
	Column 1	Column 2	Column	Mean	Sample A-B	Over-all Mean
	FID A	FID B	Precision	Value	Difference	
Sample Results	0.2161	0.2162	0.0001	0.2161	0.0003	0.2159
(g/100cc)	0.2158	0.2158	0.0000	0.2158		

Analysis Method

Refer to Blood Alcohol Method #1

Instrument Information

Instrument information is stored centrally.



Refer To Instrument Method: ALCOHOL_020725_TS.gcm

Reporting of Results		Uncertainty of Measurements (UM%): 5.00%		
Overall Mean (g/100cc)		Low	High	5 % of Mean
0.215		0.204	0.226	0.011
Reported Results				
		0.215		

Calibration and control data are stored centrally.

B

Sample Name : QC2-2
 Vial # : 63
 Data Filename : QC2-2_272025_057.gcd
 Method Filename : ALCOHOL_020725_TS.gcm
 Batch Filename : BATCH_020725_TS.gcb
 Date Acquired : 2/7/2025 7:33:20 PM
 Date Processed : 2/7/2025 7:39:20 PM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

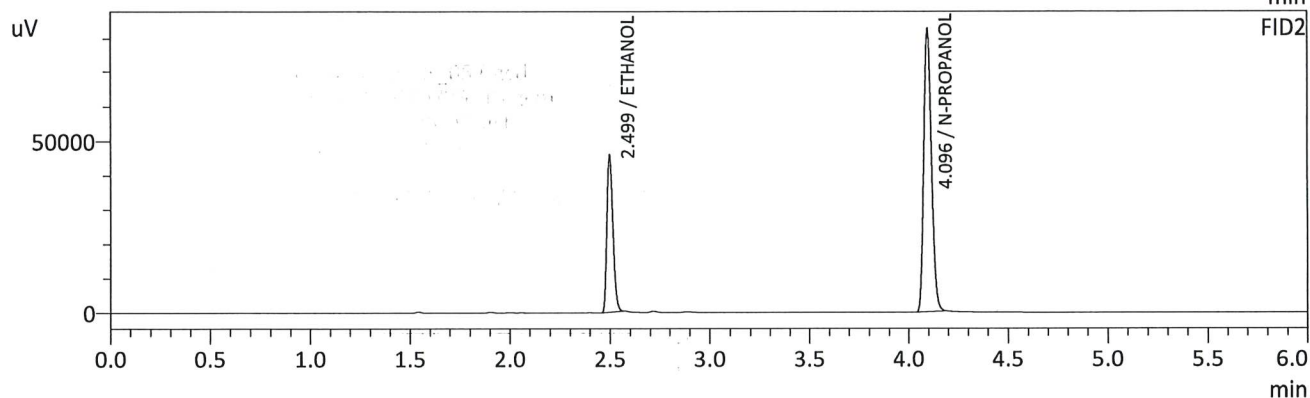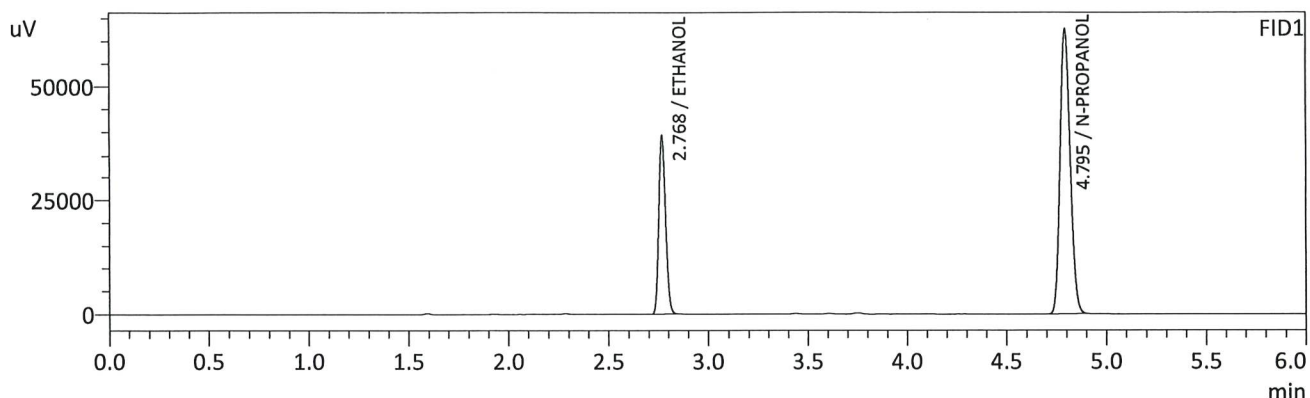

FID1



Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	0.2161	g/100cc	94643	38718
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	221340	62549
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	0.2162	g/100cc	94447	45662
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	220974	82432
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

TS

Sample Name : QC2-2-B
 Vial # : 64
 Data Filename : QC2-2-B_272025_058.gcd
 Method Filename : ALCOHOL_020725_TS.gcm
 Batch Filename : BATCH_020725_TS.gcb
 Date Acquired : 2/7/2025 7:43:10 PM
 Date Processed : 2/7/2025 7:49:11 PM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

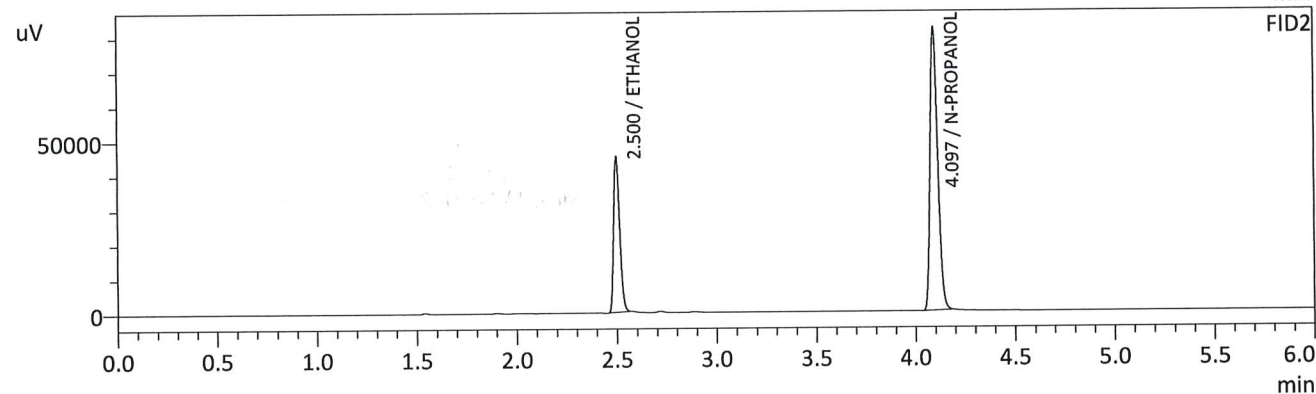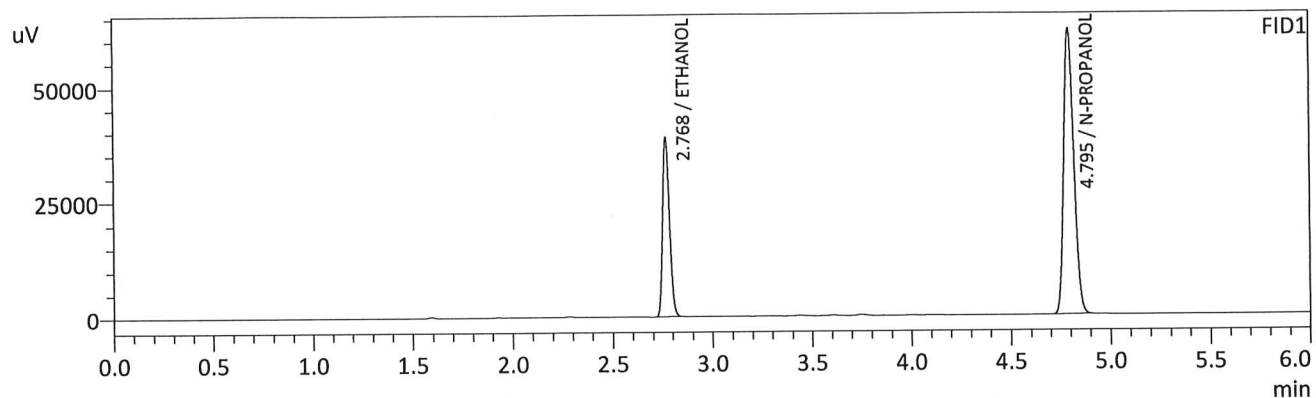

FID1



Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	0.2158	g/100cc	93618	38330
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	219242	61944
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	0.2158	g/100cc	93393	45135
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	218956	81760
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

15

Sample Name : INT STD BLK 3
 Vial # : 65
 Data Filename : INT STD BLK 3_272025_059.gcd
 Method Filename : ALCOHOL_020725_TS.gcm
 Batch Filename : BATCH_020725_TS.gcb
 Date Acquired : 2/7/2025 7:52:35 PM
 Date Processed : 2/7/2025 7:58:37 PM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

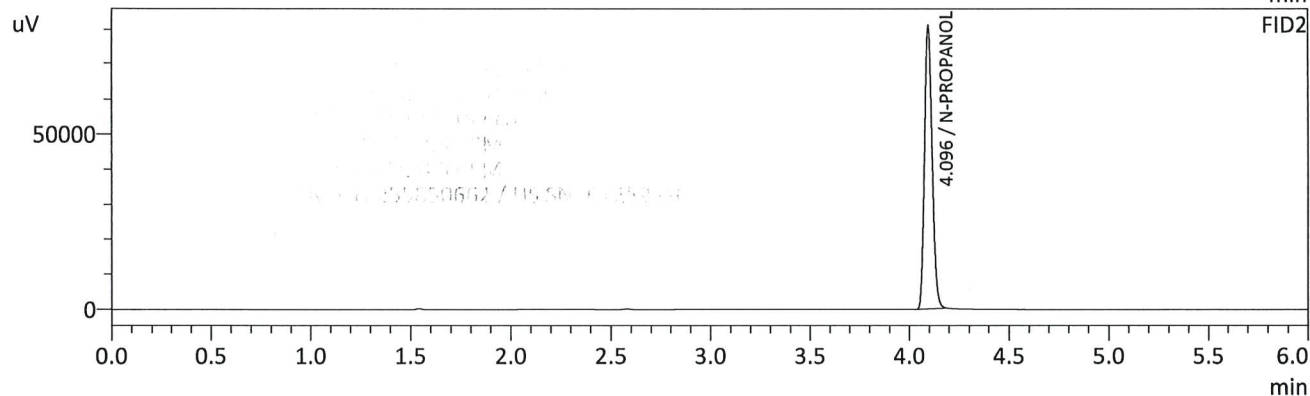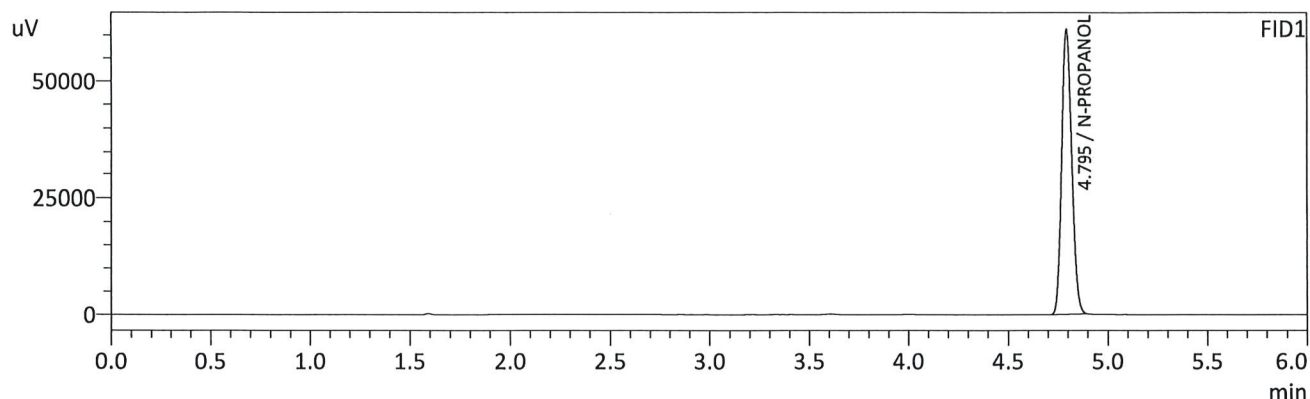



FID1

Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	215980	61117
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	215440	81033
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

Sample Name : DFE
 Vial # : 66
 Data Filename : DFE_272025_060.gcd
 Method Filename : ALCOHOL_020725_TS.gcm
 Batch Filename : BATCH_020725_TS.gcb
 Date Acquired : 2/7/2025 8:01:51 PM
 Date Processed : 2/7/2025 8:07:53 PM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

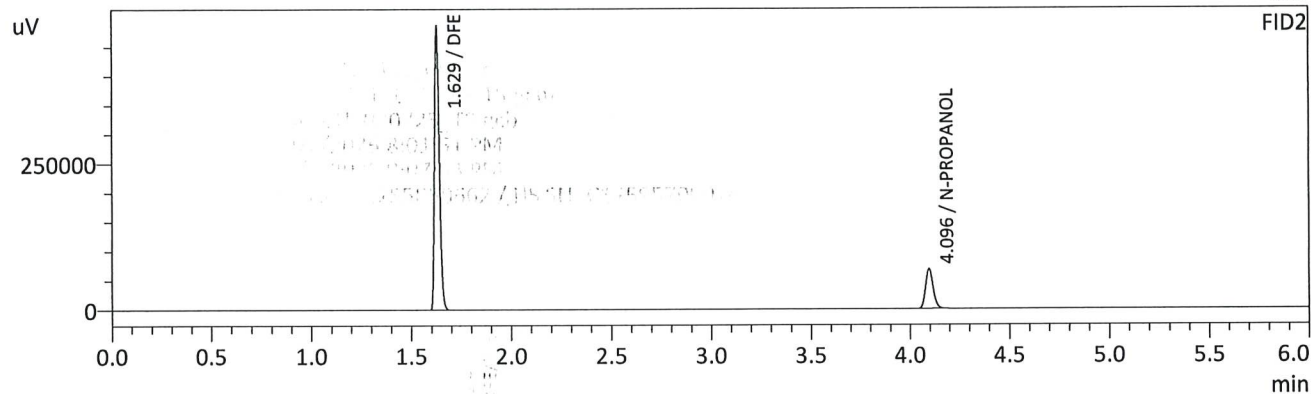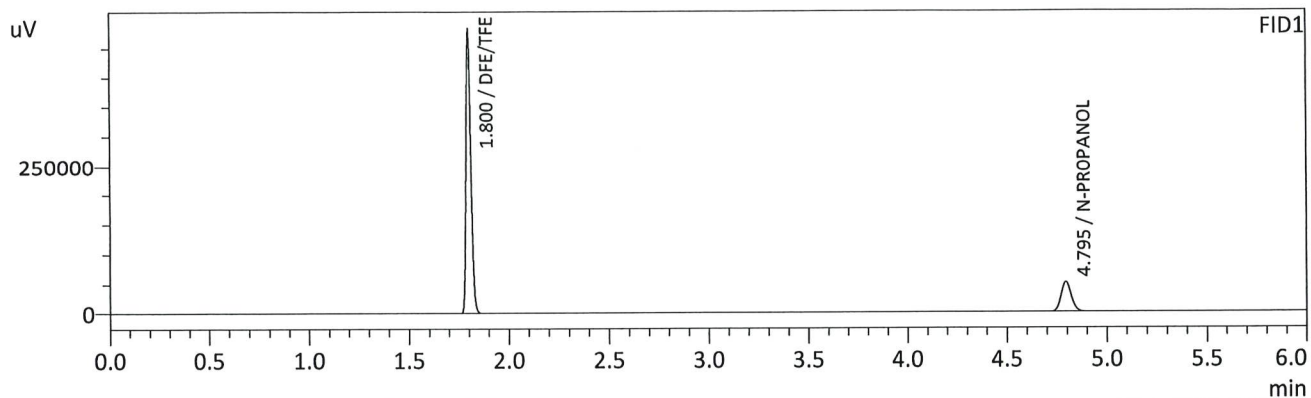

FID1



Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	182116	51659
DFE/TFE	0.0000	g/100cc	814567	480165
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	181003	68112
DFE	0.0000	g/100cc	817240	475851
TFE	--	g/100cc	--	--

15

Sample Name : INT STD BLK 4
 Vial # : 67
 Data Filename : INT STD BLK 4_272025_061.gcd
 Method Filename : ALCOHOL_020725_TS.gcm
 Batch Filename : BATCH_020725_TS.gcb
 Date Acquired : 2/7/2025 8:11:42 PM
 Date Processed : 2/7/2025 8:17:44 PM
 Instrument : GC SN- C12255850662 / HS SN- C12595700014

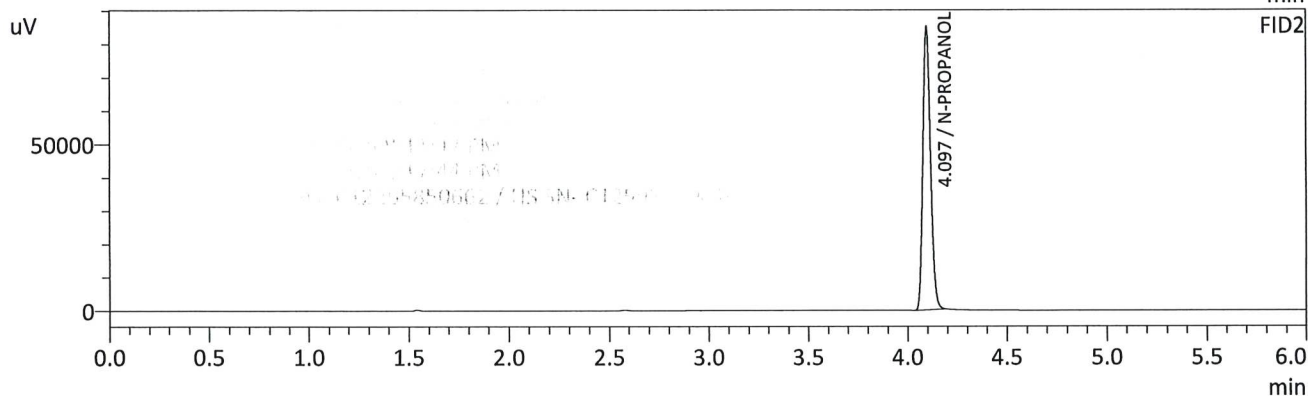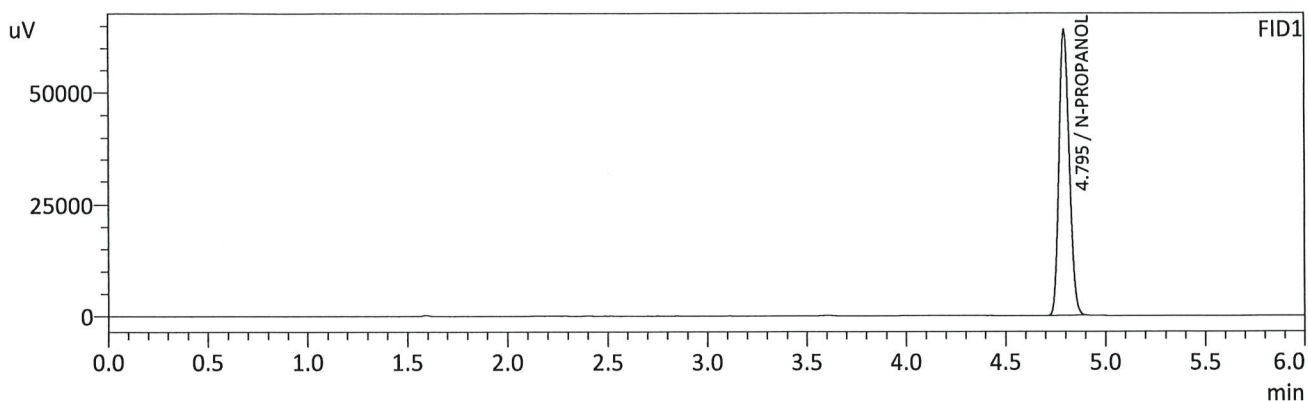

FID1

Name	Conc.	Unit	Area	Height
METHANOL	--	g/100cc	--	--
ACETALDEHYDE	--	g/100cc	--	--
ETHANOL	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	226447	63979
DFE/TFE	--	g/100cc	--	--
DME	--	g/100cc	--	--

FID2

Name	Conc.	Unit	Area	Height
ACETALDEHYDE	--	g/100cc	--	--
METHANOL	--	g/100cc	--	--
ETHANOL	--	g/100cc	--	--
ACETONE	--	g/100cc	--	--
ISOPROPYL ALCOHOL	--	g/100cc	--	--
N-PROPANOL	0.0000	g/100cc	225951	84723
DFE	--	g/100cc	--	--
TFE	--	g/100cc	--	--

TS

Region 5 Pocatello Blood Alcohol Analysis Batch Table

Shimadzu Nexis GC-2030 Serial Number: C12255850662

Shimadzu HS-20 Serial Number: C12595700014

LabSolutions Version 6.117

Copyright (C) 2008-2022 Shimadzu Corporation. All rights reserved.

Vial#	Sample Name	Sample Type	Method File	Data File	Level#
1	0.050	1:Standard:(R)	ALCOHOL_020725_TS.gcm	1-3898 - 0.050_272025_001.gcd	1
2	0.100	1:Standard:(R)	ALCOHOL_020725_TS.gcm	1-3899 - 0.100_272025_002.gcd	2
3	0.200	1:Standard:(R)	ALCOHOL_020725_TS.gcm	1-3900 - 0.200_272025_003.gcd	3
4	0.300	1:Standard:(R)	ALCOHOL_020725_TS.gcm	1-3901 - 0.300_272025_004.gcd	4
5	0.500	1:Standard:(R)	ALCOHOL_020725_TS.gcm	1-3902 - 0.500_272025_005.gcd	5
6	INT STD BLK 1	0:Unknown	ALCOHOL_020725_TS.gcm	1-3903 - INT STD BLK 1_272025_006.gcd	0
7	MULTI-COMP MIX	0:Unknown	ALCOHOL_020725_TS.gcm	3904 - MULTI-COMP MIX_272025_001.gcd	1
8	INT STD BLK 2	0:Unknown	ALCOHOL_020725_TS.gcm	1-3905 - INT STD BLK 2_272025_002.gcd	0
9	QC1-1	0:Unknown	ALCOHOL_020725_TS.gcm	1-3906 - QC1-1_272025_003.gcd	0
10	QC1-1-B	0:Unknown	ALCOHOL_020725_TS.gcm	1-3907 - QC1-1-B_272025_004.gcd	0
11	0.08 QA	0:Unknown	ALCOHOL_020725_TS.gcm	1-3908 - 0.08 QA_272025_005.gcd	0
12	0.08 QA - B	0:Unknown	ALCOHOL_020725_TS.gcm	1-3909 - 0.08 QA - B_272025_006.gcd	0
13	P2025-0069-1	0:Unknown	ALCOHOL_020725_TS.gcm	1-3910 - P2025-0069-1_272025_007.gcd	0
14	P2025-0069-1-B	0:Unknown	ALCOHOL_020725_TS.gcm	1-3911 - P2025-0069-1-B_272025_008.gcd	0
15	P2025-0078-1	0:Unknown	ALCOHOL_020725_TS.gcm	1-3912 - P2025-0078-1_272025_009.gcd	0
16	P2025-0078-1-B	0:Unknown	ALCOHOL_020725_TS.gcm	1-3913 - P2025-0078-1-B_272025_010.gcd	0
17	P2025-0079-1	0:Unknown	ALCOHOL_020725_TS.gcm	1-3914 - P2025-0079-1_272025_011.gcd	0
18	P2025-0079-1-B	0:Unknown	ALCOHOL_020725_TS.gcm	1-3915 - P2025-0079-1-B_272025_012.gcd	0
19	P2025-0080-1	0:Unknown	ALCOHOL_020725_TS.gcm	1-3916 - P2025-0080-1_272025_013.gcd	0
20	P2025-0080-1-B	0:Unknown	ALCOHOL_020725_TS.gcm	1-3917 - P2025-0080-1-B_272025_014.gcd	0
21	P2025-0083-1	0:Unknown	ALCOHOL_020725_TS.gcm	1-3918 - P2025-0083-1_272025_015.gcd	0
22	P2025-0083-1-B	0:Unknown	ALCOHOL_020725_TS.gcm	1-3919 - P2025-0083-1-B_272025_016.gcd	0
23	P2025-0084-1	0:Unknown	ALCOHOL_020725_TS.gcm	1-3920 - P2025-0084-1_272025_017.gcd	0
24	P2025-0084-1-B	0:Unknown	ALCOHOL_020725_TS.gcm	1-3921 - P2025-0084-1-B_272025_018.gcd	0
25	P2025-0091-2	0:Unknown	ALCOHOL_020725_TS.gcm	1-3922 - P2025-0091-2_272025_019.gcd	0
26	P2025-0091-2-B	0:Unknown	ALCOHOL_020725_TS.gcm	1-3923 - P2025-0091-2-B_272025_020.gcd	0
27	P2025-0097-1	0:Unknown	ALCOHOL_020725_TS.gcm	1-3924 - P2025-0097-1_272025_021.gcd	0
28	P2025-0097-1-B	0:Unknown	ALCOHOL_020725_TS.gcm	1-3925 - P2025-0097-1-B_272025_022.gcd	0
29	P2025-0098-1	0:Unknown	ALCOHOL_020725_TS.gcm	1-3926 - P2025-0098-1_272025_023.gcd	0
30	P2025-0098-1-B	0:Unknown	ALCOHOL_020725_TS.gcm	1-3927 - P2025-0098-1-B_272025_024.gcd	0
31	QC2-1	0:Unknown	ALCOHOL_020725_TS.gcm	1-3928 - QC2-1_272025_025.gcd	0
32	QC2-1-B	0:Unknown	ALCOHOL_020725_TS.gcm	1-3929 - QC2-1-B_272025_026.gcd	0
33	P2025-0112-1	0:Unknown	ALCOHOL_020725_TS.gcm	1-3930 - P2025-0112-1_272025_027.gcd	0
34	P2025-0112-1-B	0:Unknown	ALCOHOL_020725_TS.gcm	1-3931 - P2025-0112-1-B_272025_028.gcd	0
35	P2025-0114-1	0:Unknown	ALCOHOL_020725_TS.gcm	1-3932 - P2025-0114-1_272025_029.gcd	0
36	P2025-0114-1-B	0:Unknown	ALCOHOL_020725_TS.gcm	1-3933 - P2025-0114-1-B_272025_030.gcd	0
37	P2025-0124-1	0:Unknown	ALCOHOL_020725_TS.gcm	1-3934 - P2025-0124-1_272025_031.gcd	0
38	P2025-0124-1-B	0:Unknown	ALCOHOL_020725_TS.gcm	1-3935 - P2025-0124-1-B_272025_032.gcd	0
39	P2025-0134-1	0:Unknown	ALCOHOL_020725_TS.gcm	1-3936 - P2025-0134-1_272025_033.gcd	0
40	P2025-0134-1-B	0:Unknown	ALCOHOL_020725_TS.gcm	1-3937 - P2025-0134-1-B_272025_034.gcd	0
41	P2025-0136-1	0:Unknown	ALCOHOL_020725_TS.gcm	1-3938 - P2025-0136-1_272025_035.gcd	0
42	P2025-0136-1-B	0:Unknown	ALCOHOL_020725_TS.gcm	1-3939 - P2025-0136-1-B_272025_036.gcd	0
43	P2025-0149-1	0:Unknown	ALCOHOL_020725_TS.gcm	1-3940 - P2025-0149-1_272025_037.gcd	0
44	P2025-0149-1-B	0:Unknown	ALCOHOL_020725_TS.gcm	1-3941 - P2025-0149-1-B_272025_038.gcd	0
45	P2025-0155-1	0:Unknown	ALCOHOL_020725_TS.gcm	1-3942 - P2025-0155-1_272025_039.gcd	0
46	P2025-0155-1-B	0:Unknown	ALCOHOL_020725_TS.gcm	1-3943 - P2025-0155-1-B_272025_040.gcd	0
47	P2025-0156-1	0:Unknown	ALCOHOL_020725_TS.gcm	1-3944 - P2025-0156-1_272025_041.gcd	0
48	P2025-0156-1-B	0:Unknown	ALCOHOL_020725_TS.gcm	1-3945 - P2025-0156-1-B_272025_042.gcd	0
49	P2025-0158-1	0:Unknown	ALCOHOL_020725_TS.gcm	1-3946 - P2025-0158-1_272025_043.gcd	0
50	P2025-0158-1-B	0:Unknown	ALCOHOL_020725_TS.gcm	1-3947 - P2025-0158-1-B_272025_044.gcd	0
51	P2025-0159-1	0:Unknown	ALCOHOL_020725_TS.gcm	1-3948 - P2025-0159-1_272025_045.gcd	0
52	P2025-0159-1-B	0:Unknown	ALCOHOL_020725_TS.gcm	1-3949 - P2025-0159-1-B_272025_046.gcd	0
53	QC1-2	0:Unknown	ALCOHOL_020725_TS.gcm	1-3950 - QC1-2_272025_047.gcd	0
54	QC1-2-B	0:Unknown	ALCOHOL_020725_TS.gcm	1-3951 - QC1-2-B_272025_048.gcd	0
55	P2025-0167-1	0:Unknown	ALCOHOL_020725_TS.gcm	1-3952 - P2025-0167-1_272025_049.gcd	0
56	P2025-0167-1-B	0:Unknown	ALCOHOL_020725_TS.gcm	1-3953 - P2025-0167-1-B_272025_050.gcd	0
57	P2025-0168-1	0:Unknown	ALCOHOL_020725_TS.gcm	1-3954 - P2025-0168-1_272025_051.gcd	0
58	P2025-0168-1-B	0:Unknown	ALCOHOL_020725_TS.gcm	1-3955 - P2025-0168-1-B_272025_052.gcd	0

Vial#	Sample Name	Sample Type	Method File	Data File	Level#
59	P2025-0185-1	0:Unknown	ALCOHOL_020725_TS.gcm	1-3956 - P2025-0185-1_272025_053.gcd	0
60	P2025-0185-1-B	0:Unknown	ALCOHOL_020725_TS.gcm	1-3957 - P2025-0185-1-B_272025_054.gcd	0
61	P2025-0187-1	0:Unknown	ALCOHOL_020725_TS.gcm	1-3958 - P2025-0187-1_272025_055.gcd	0
62	P2025-0187-1-B	0:Unknown	ALCOHOL_020725_TS.gcm	1-3959 - P2025-0187-1-B_272025_056.gcd	0
63	QC2-2	0:Unknown	ALCOHOL_020725_TS.gcm	1-3960 - QC2-2_272025_057.gcd	0
64	QC2-2-B	0:Unknown	ALCOHOL_020725_TS.gcm	1-3961 - QC2-2-B_272025_058.gcd	0
65	INT STD BLK 3	0:Unknown	ALCOHOL_020725_TS.gcm	1-3962 - INT STD BLK 3_272025_059.gcd	0
66	DFE	0:Unknown	ALCOHOL_020725_TS.gcm	1-3963 - DFE_272025_060.gcd	0
67	INT STD BLK 4	0:Unknown	ALCOHOL_020725_TS.gcm	1-3964 - INT STD BLK 4_272025_061.gcd	0